



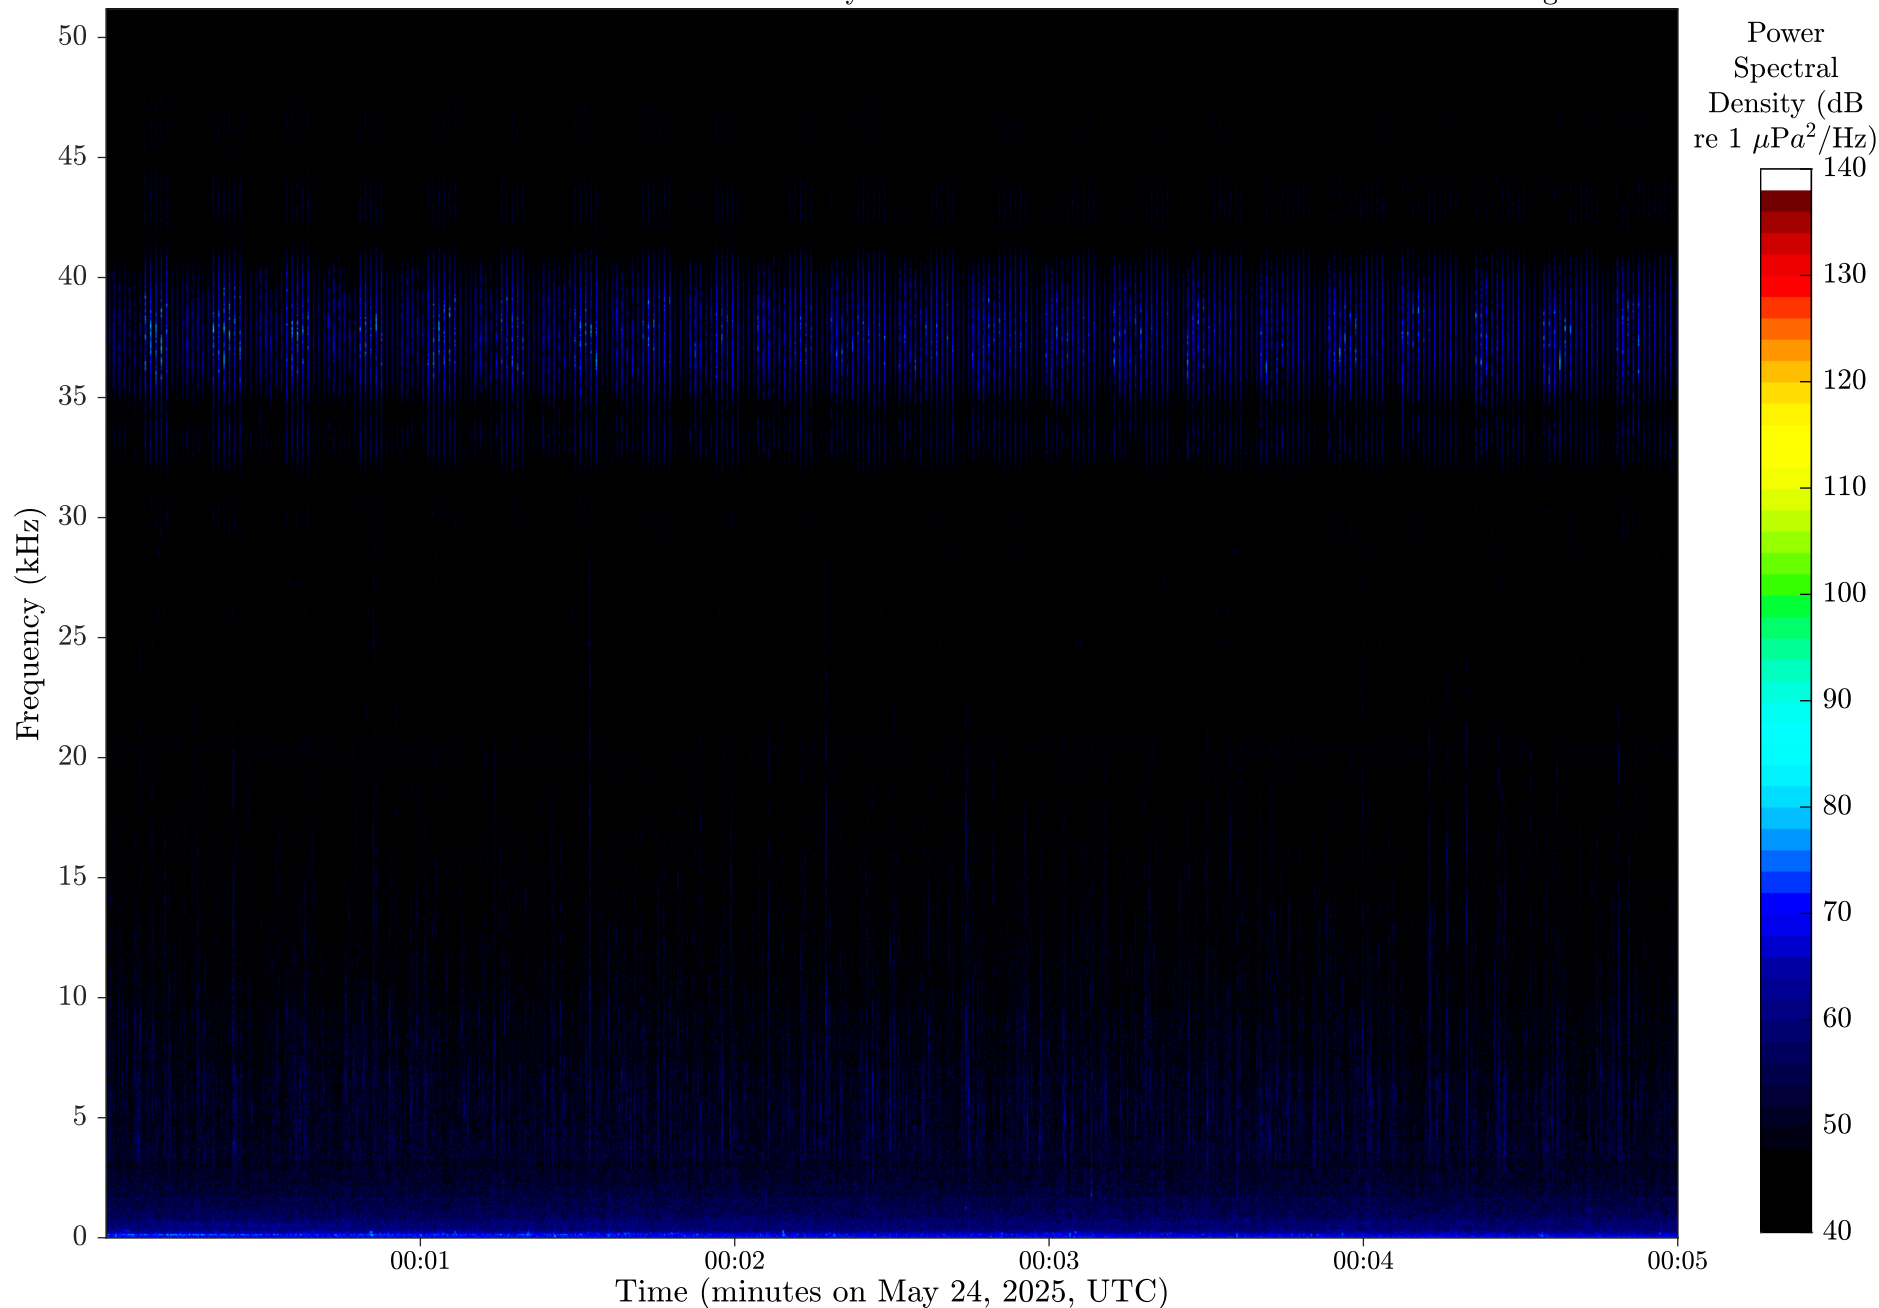


Comments: 31.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:08:05 UTC

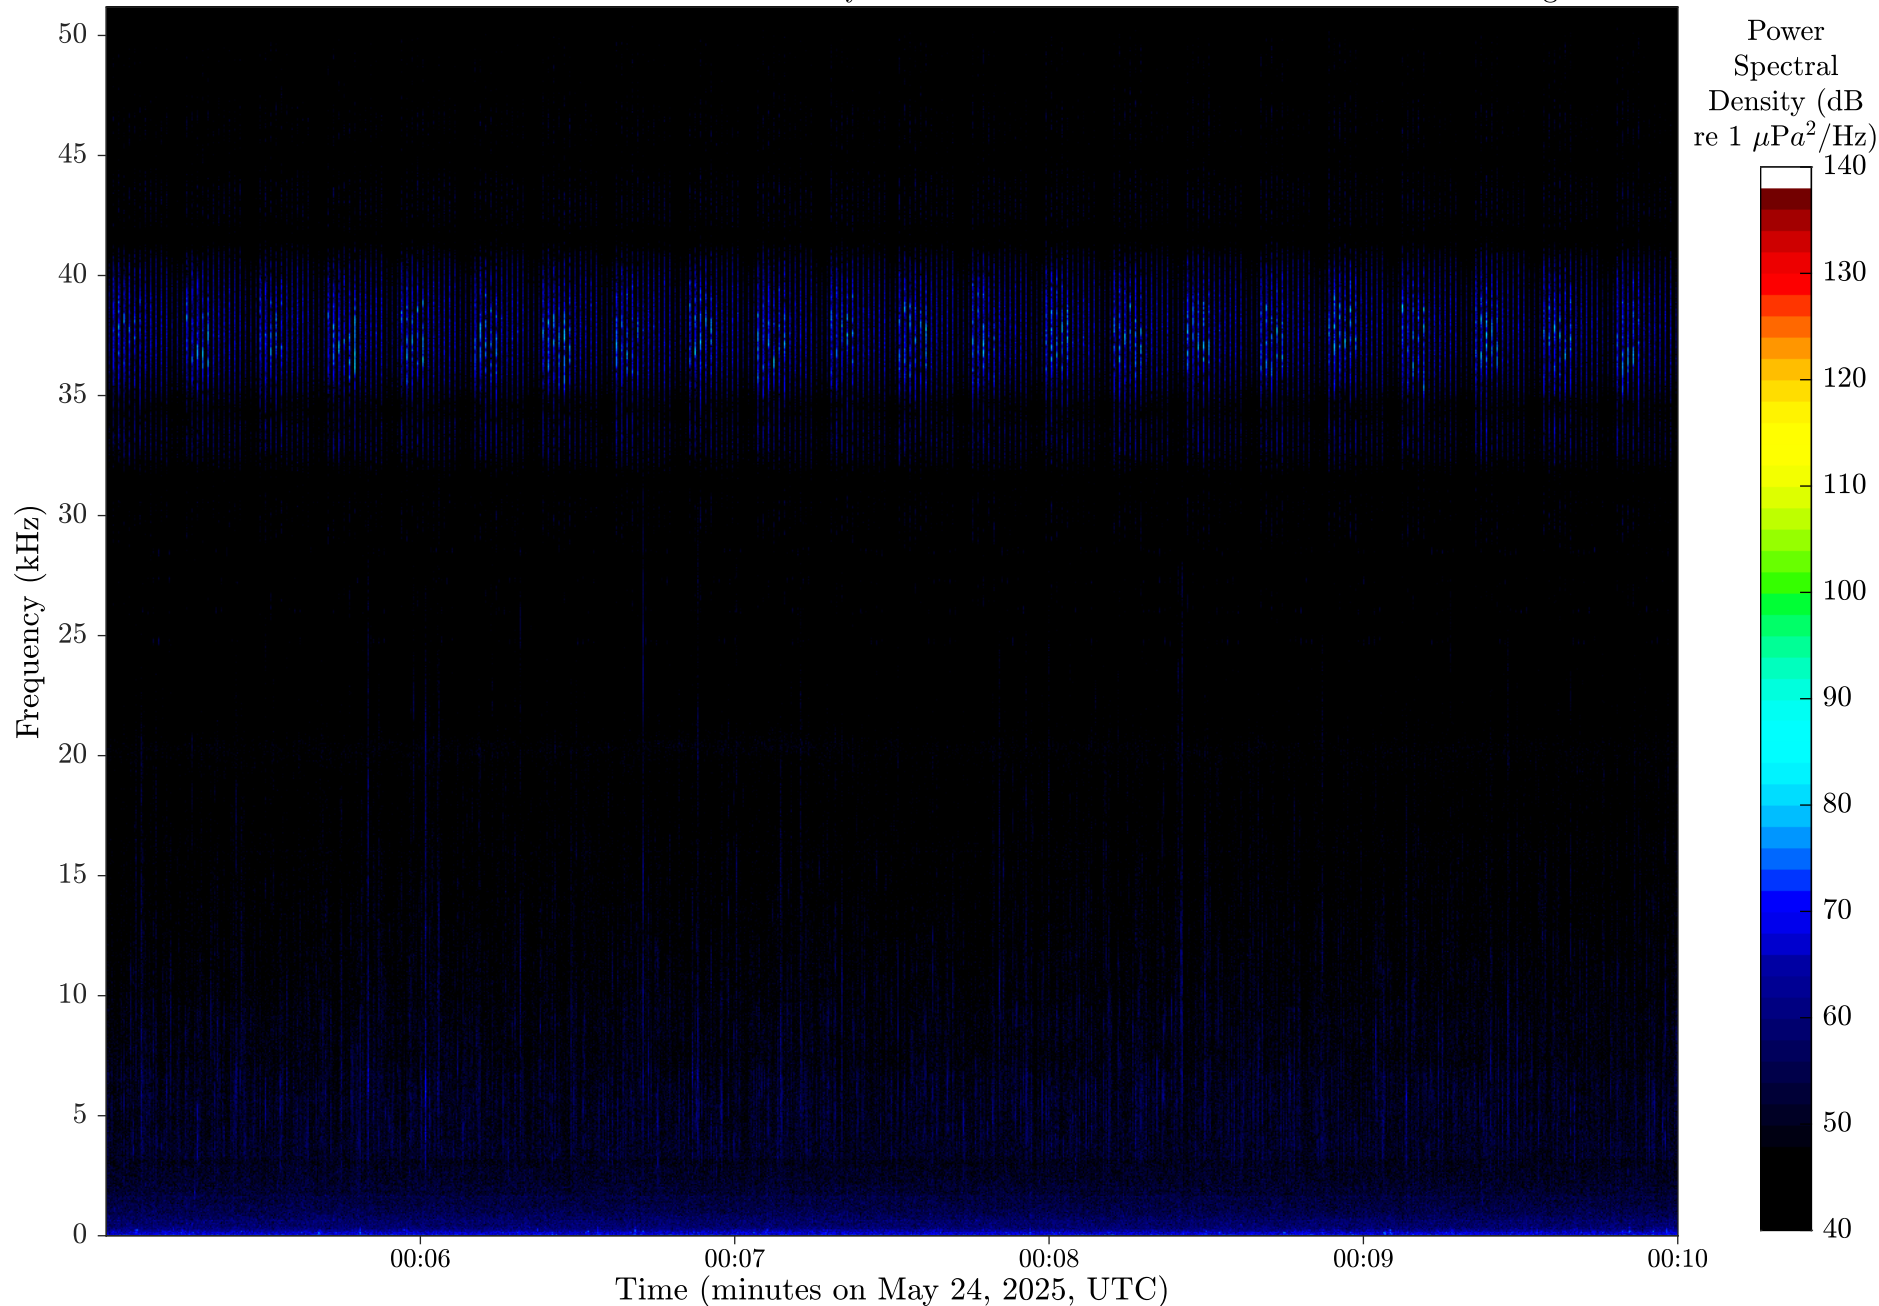


Comments: 32.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:08:13 UTC

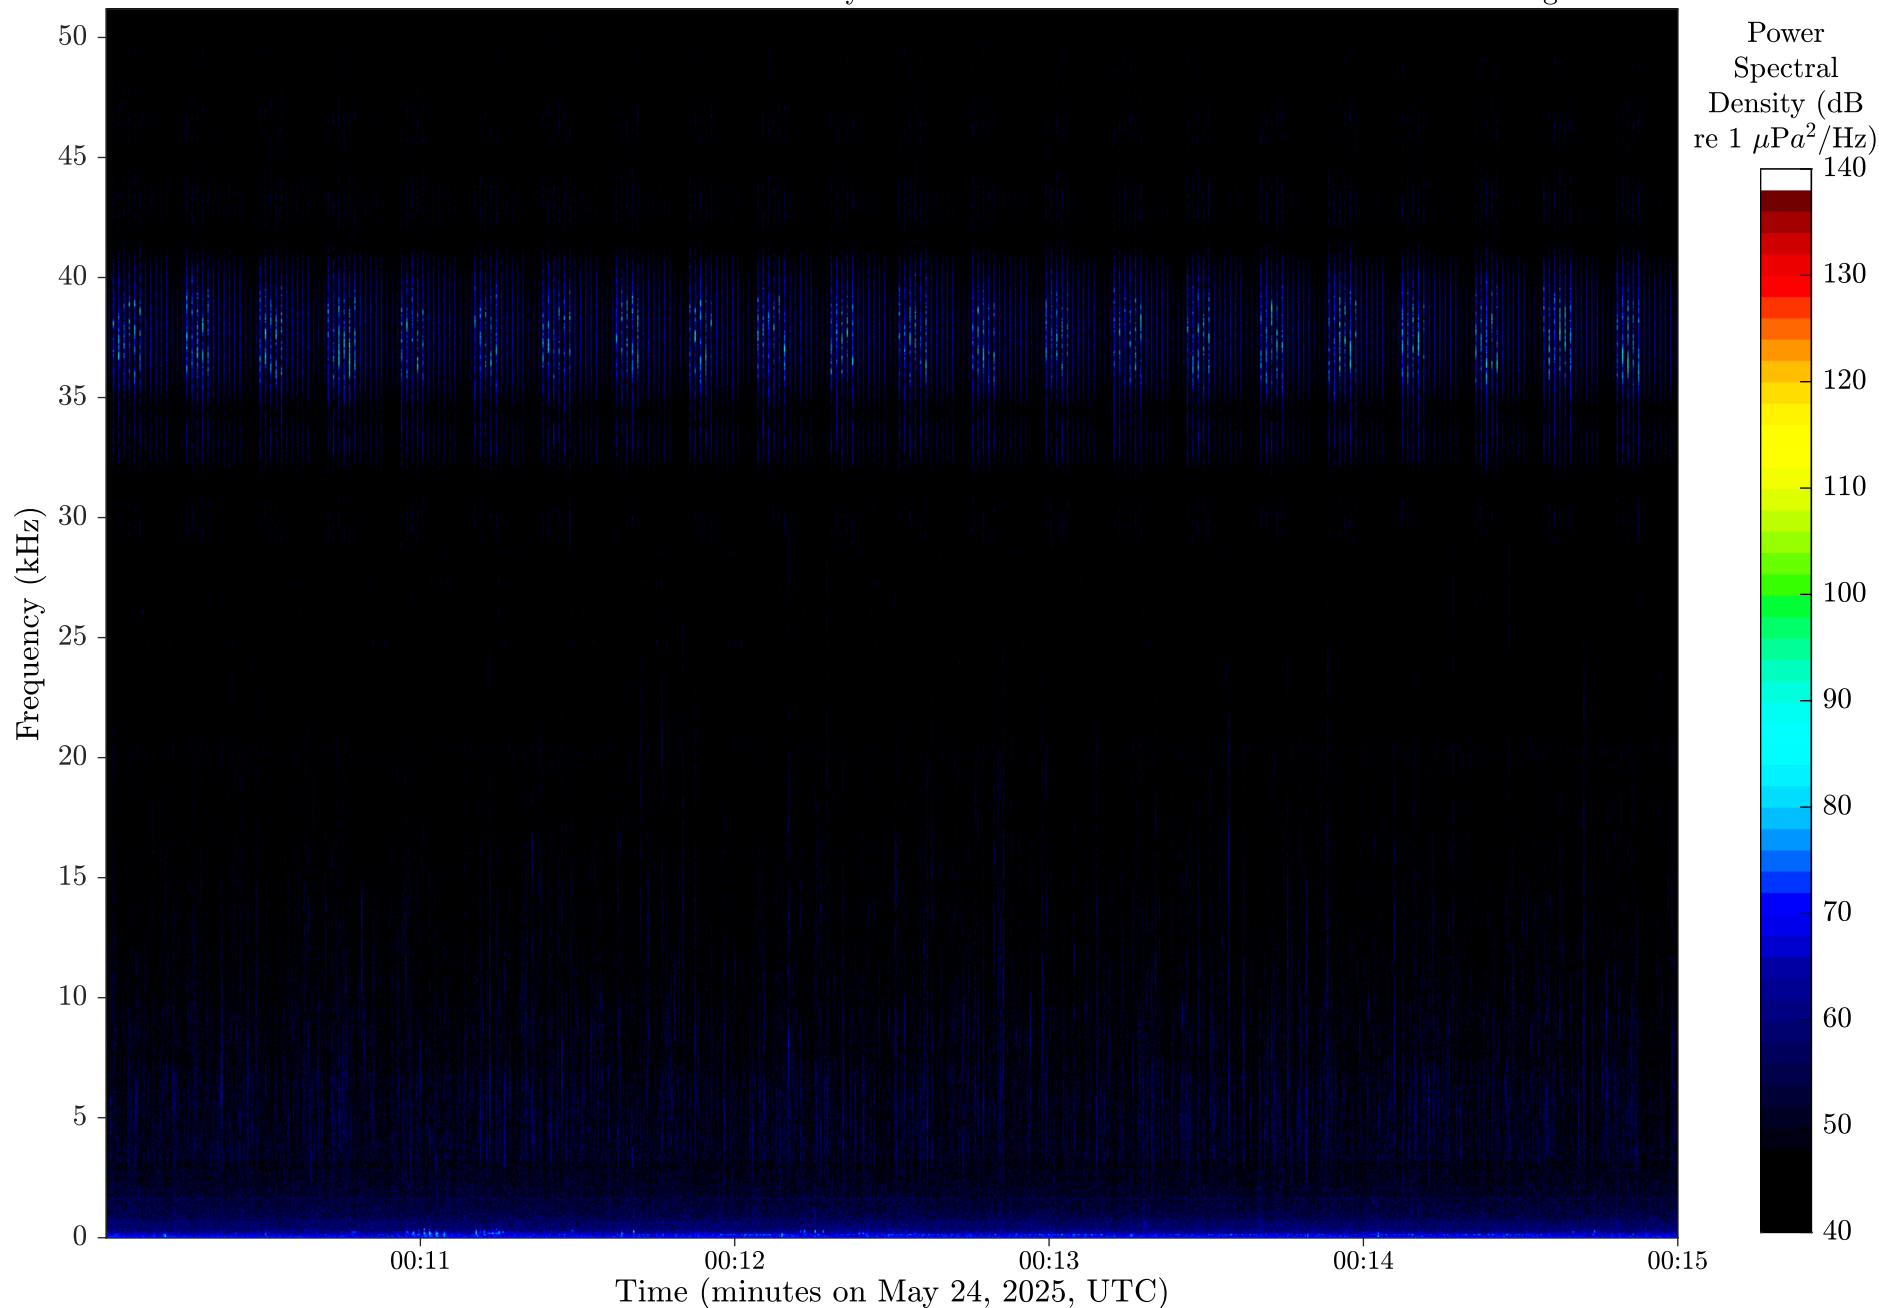


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:08:21 UTC

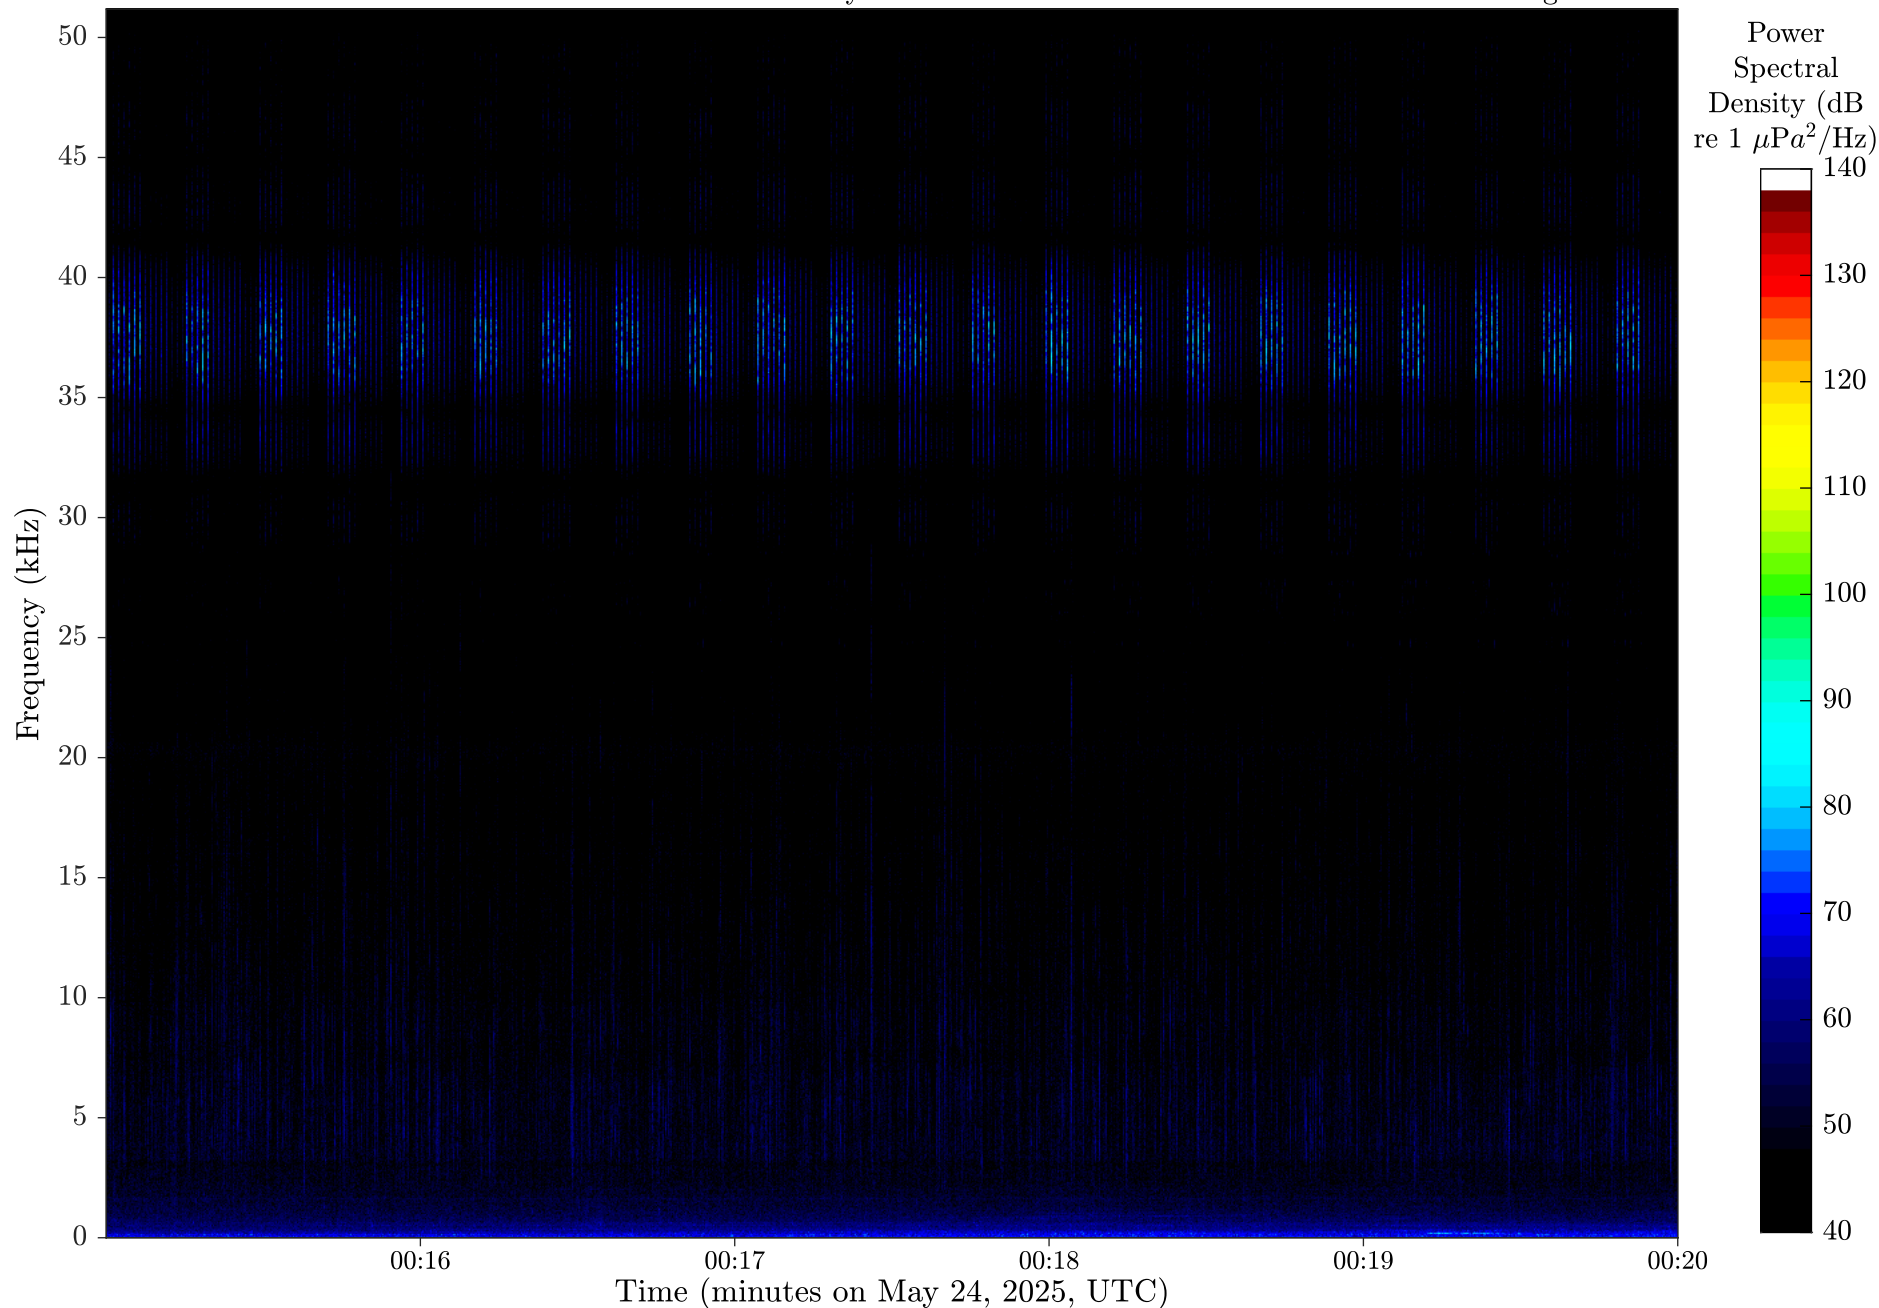


Comments: 35.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:08:29 UTC

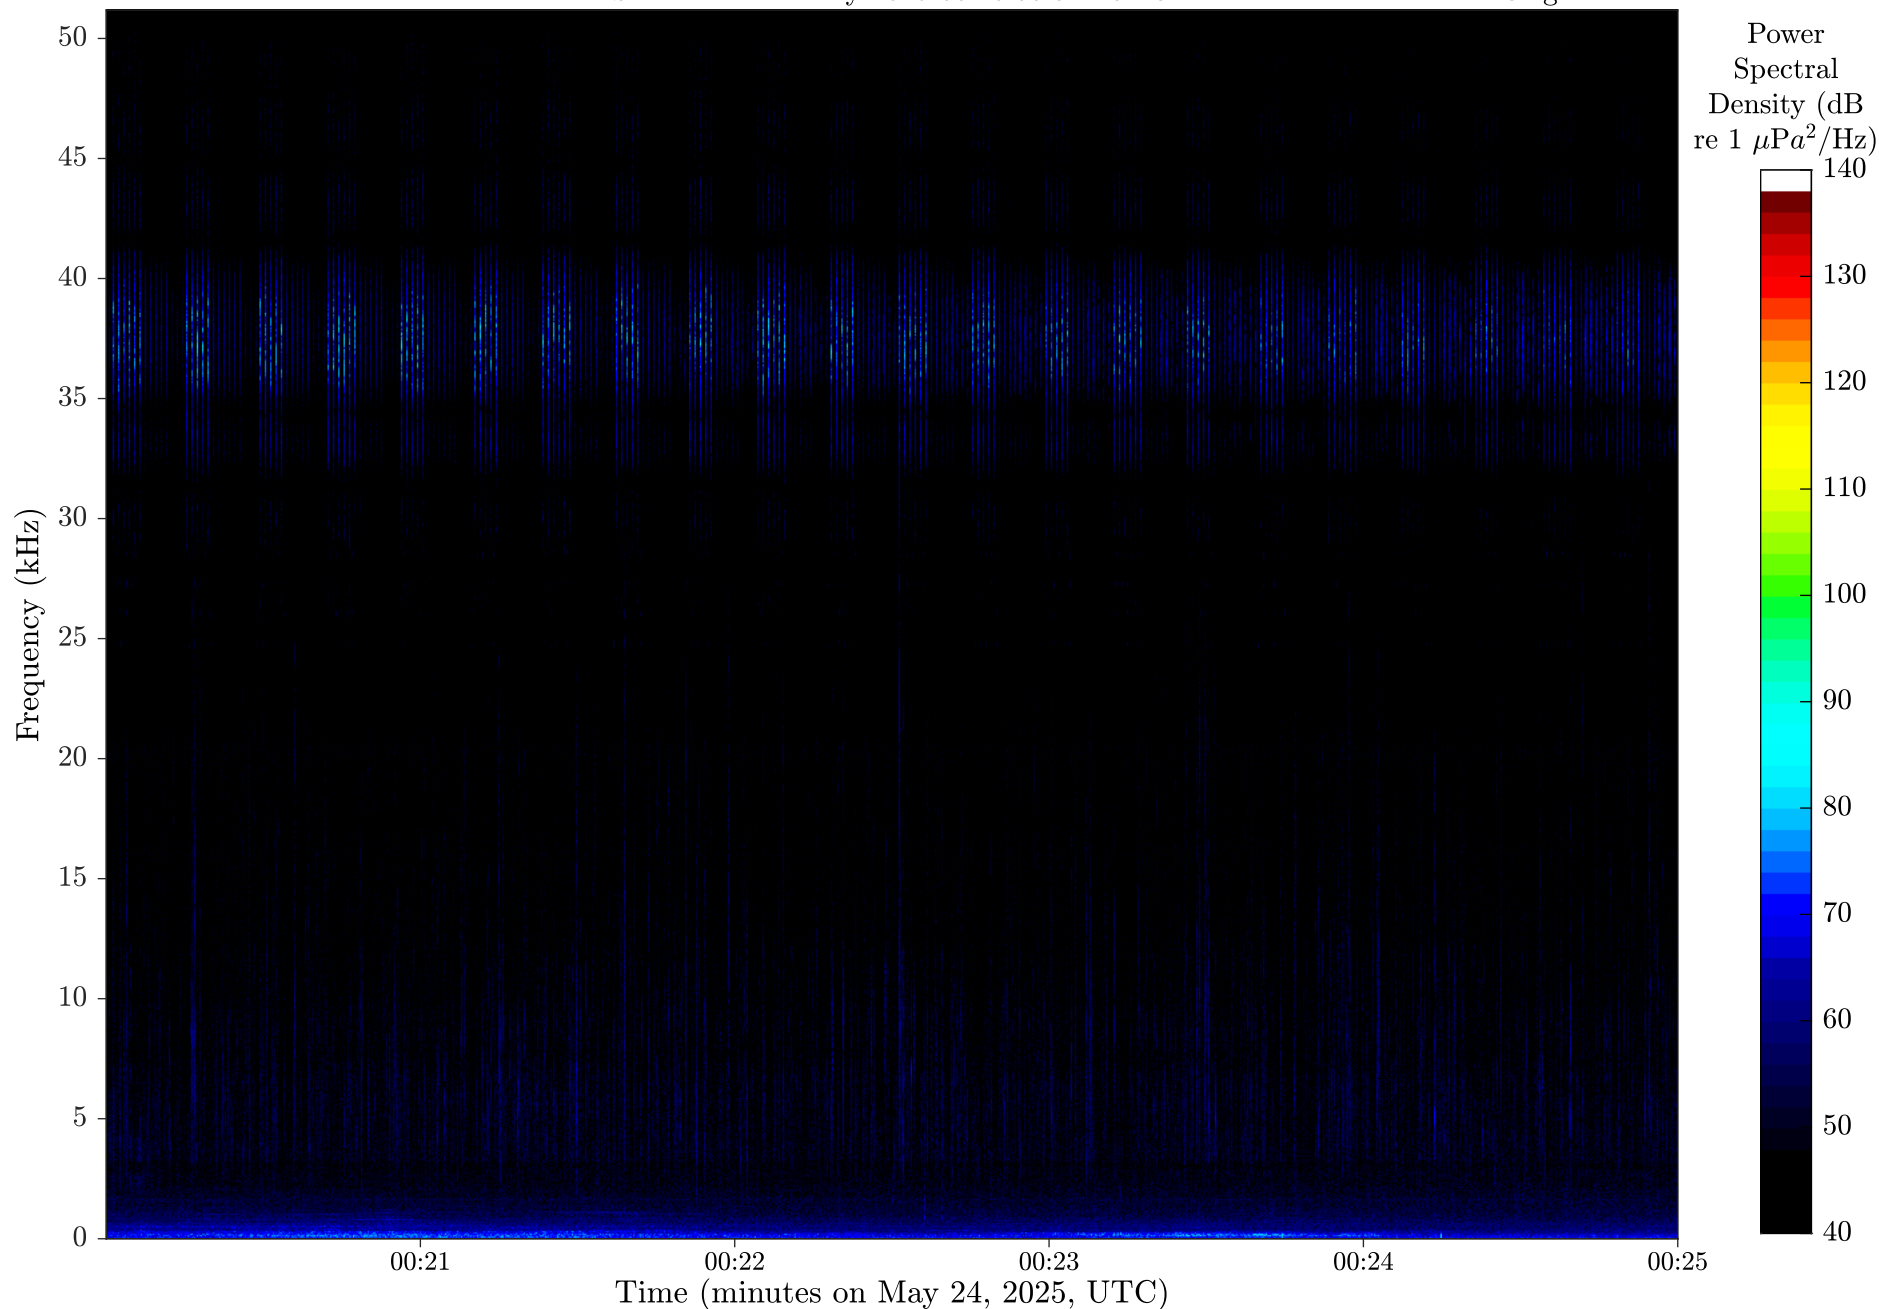

Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:08:36 UTC

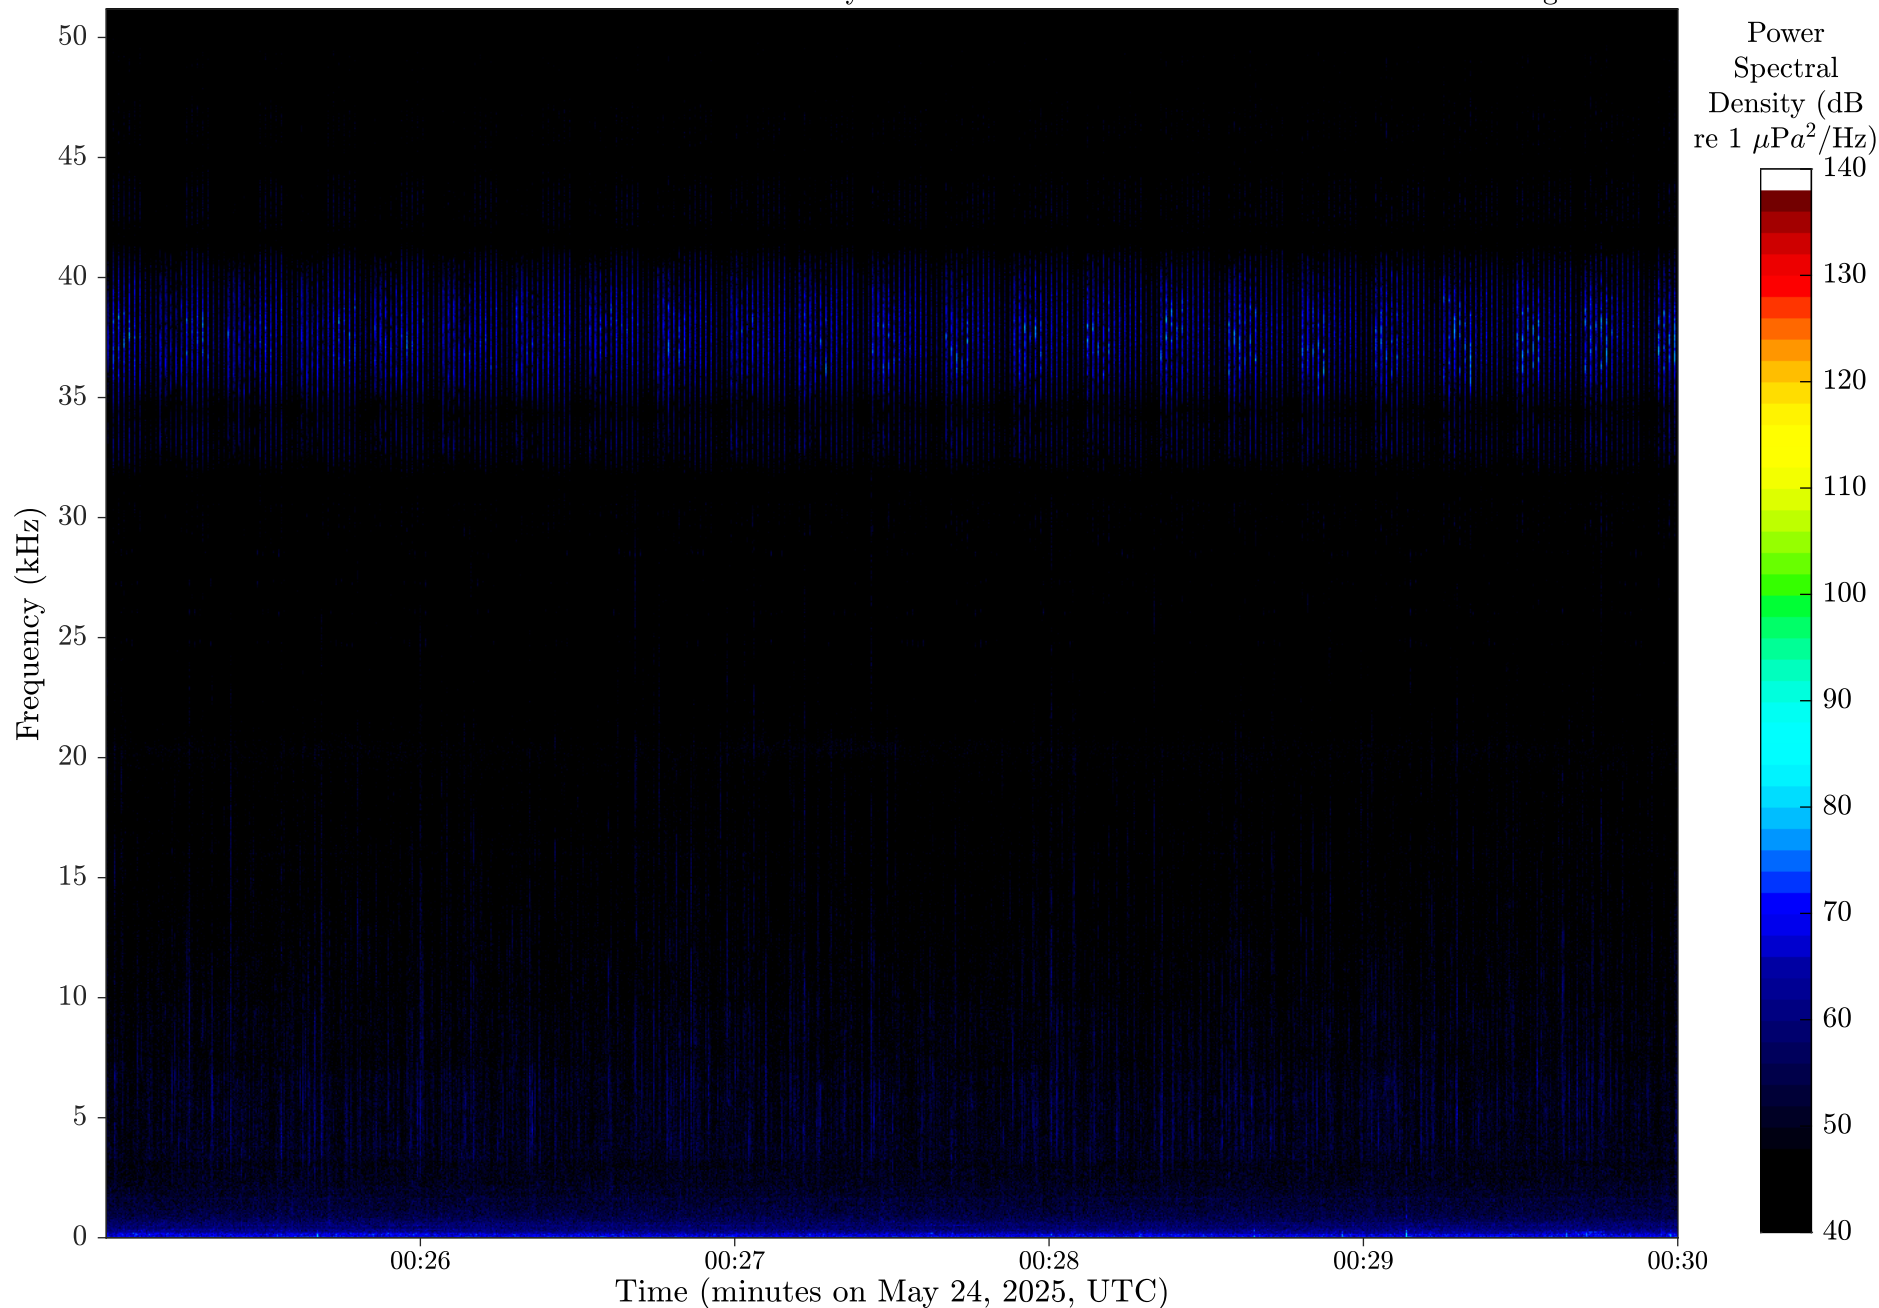

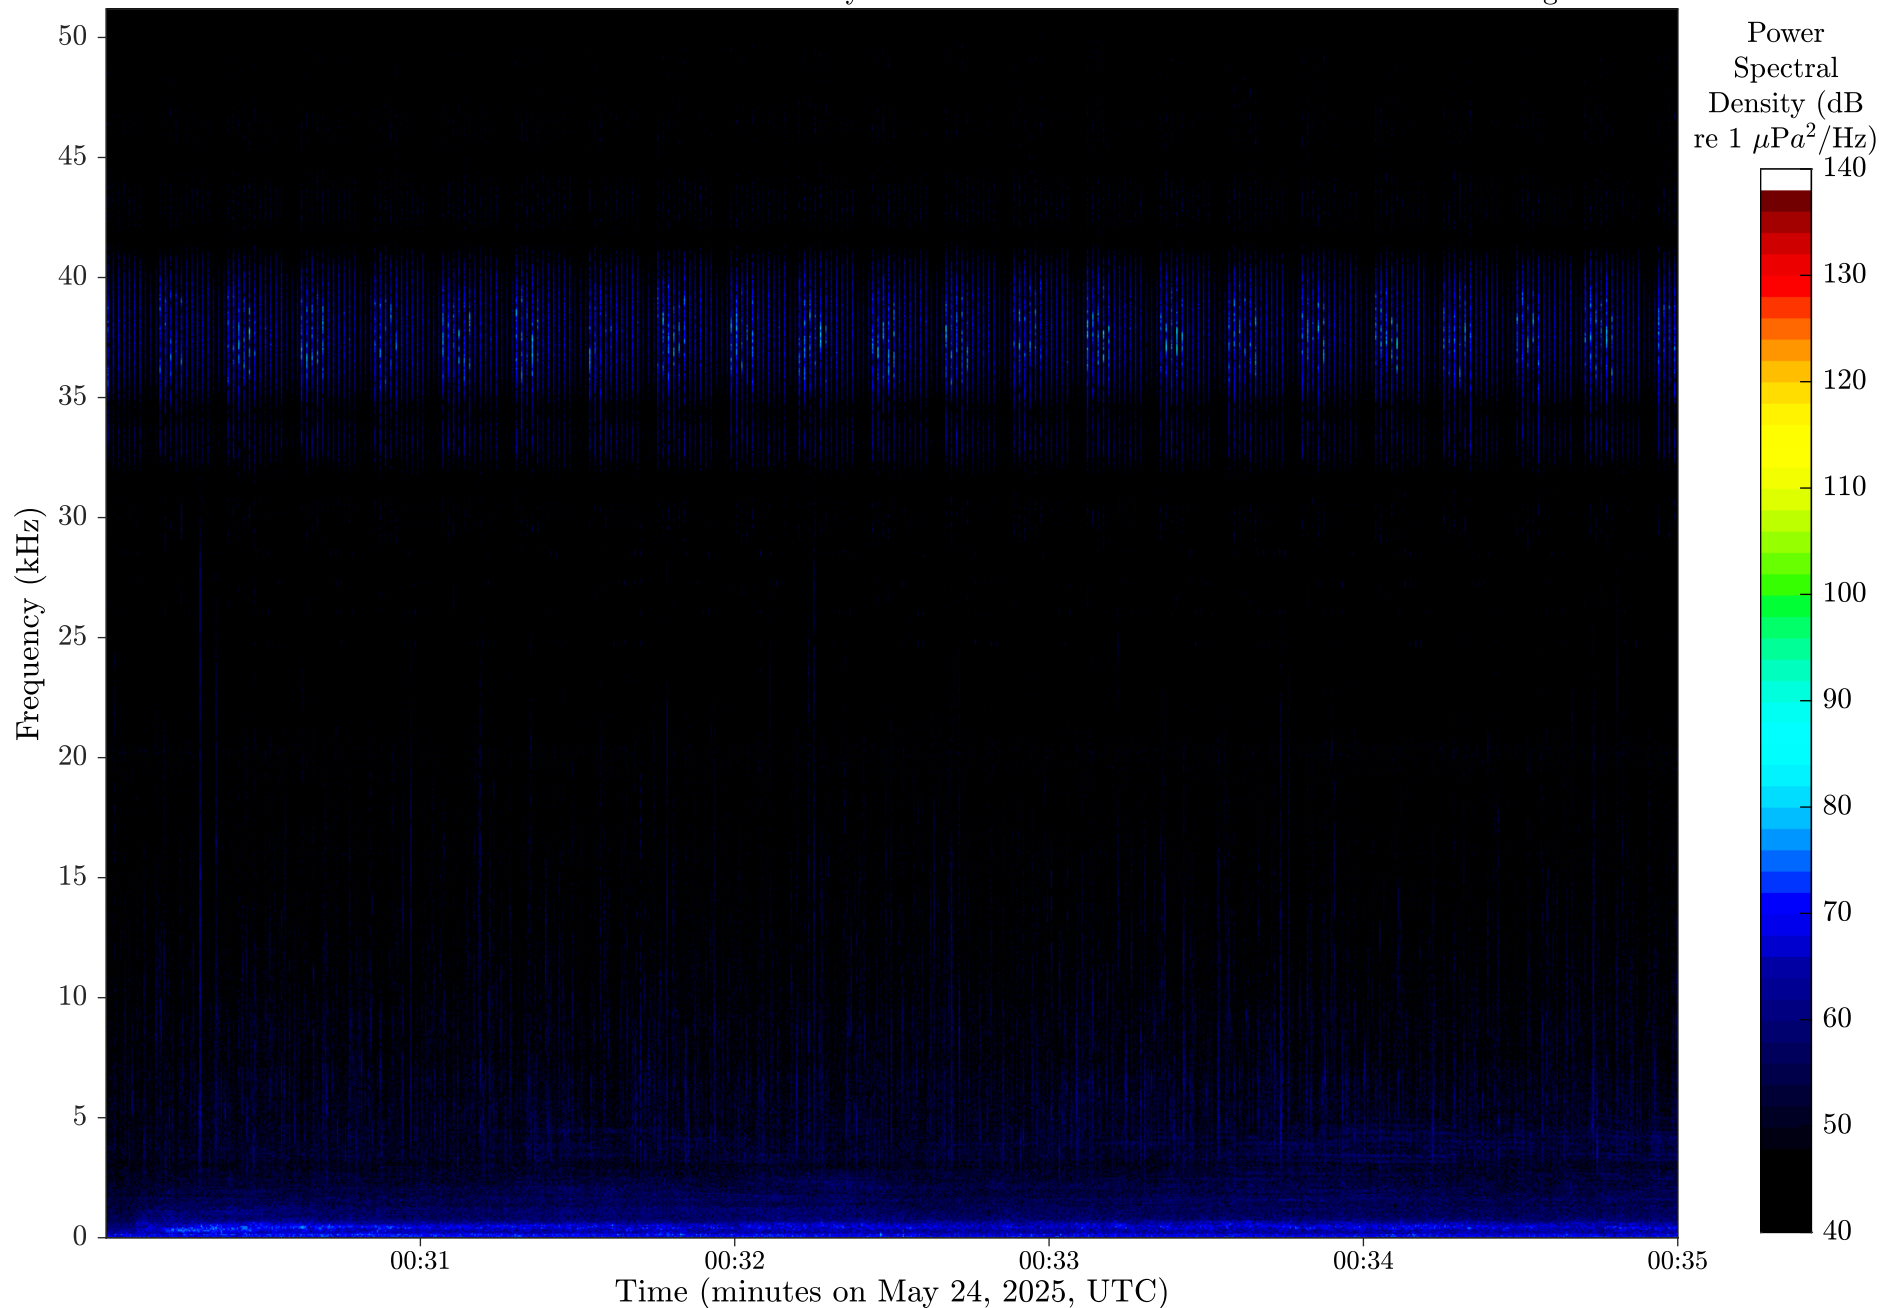


Comments: 33.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:08:50 UTC

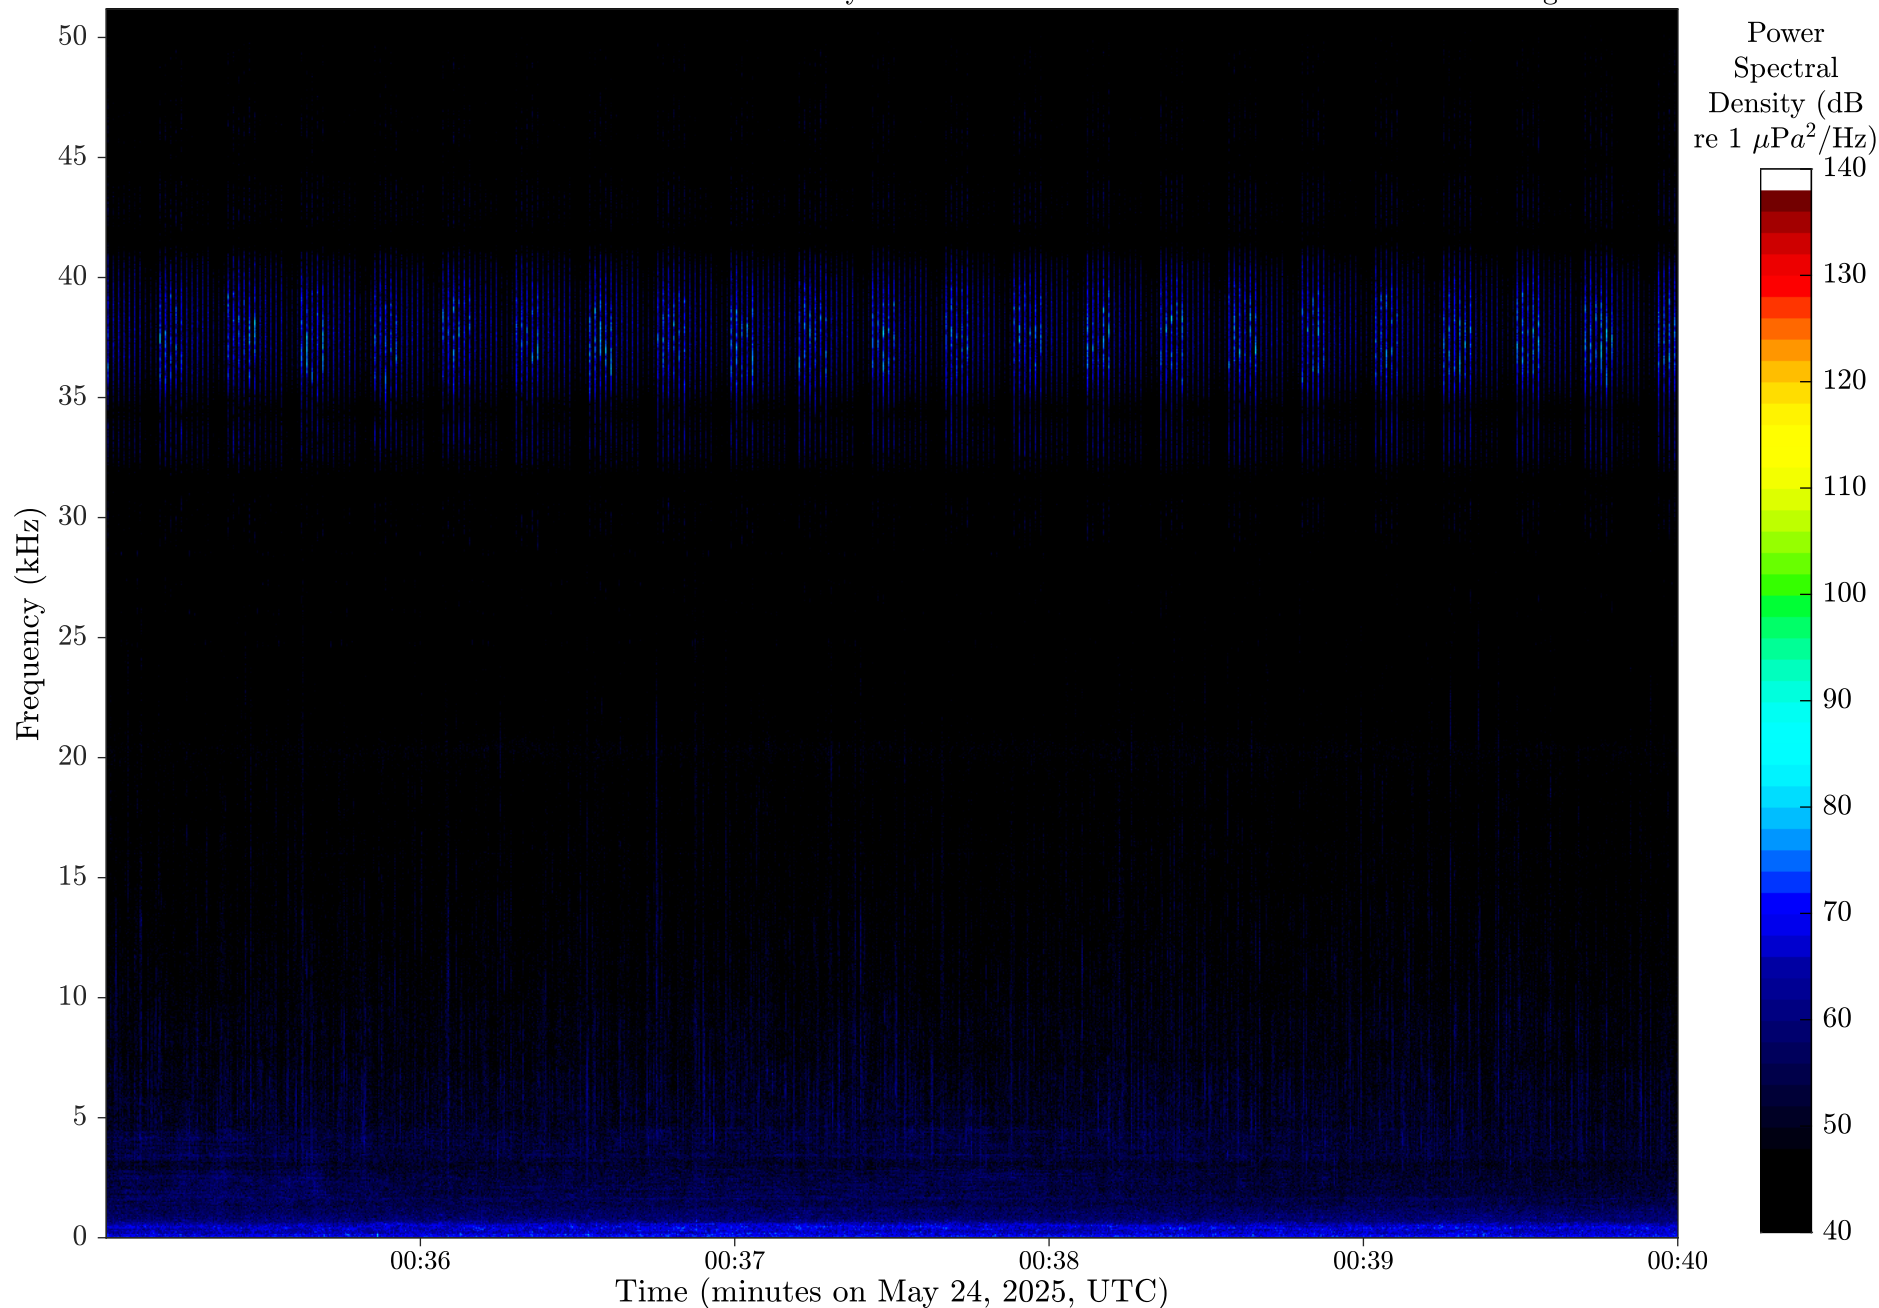

Comments: 34.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:08:57 UTC

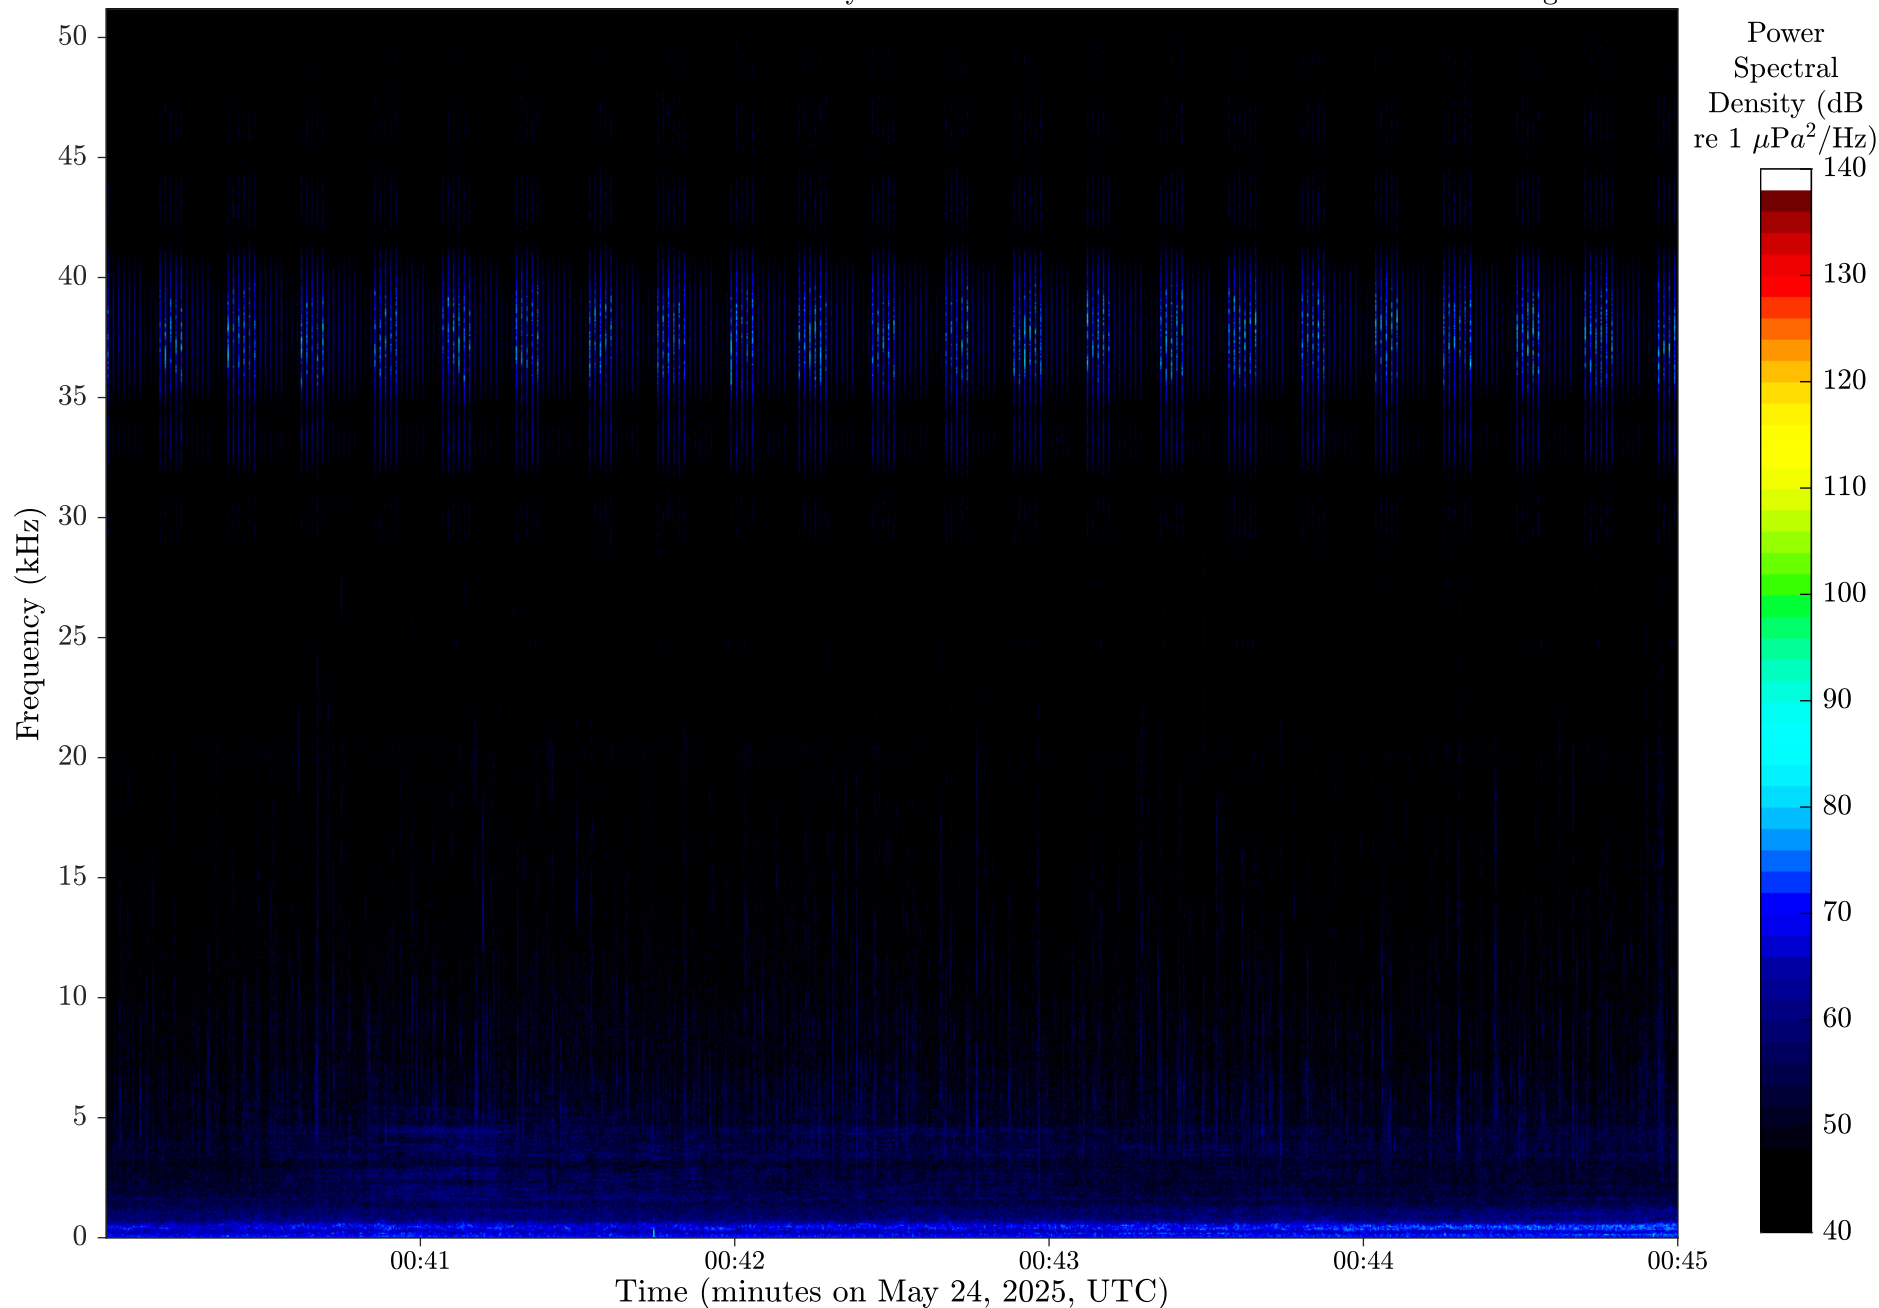

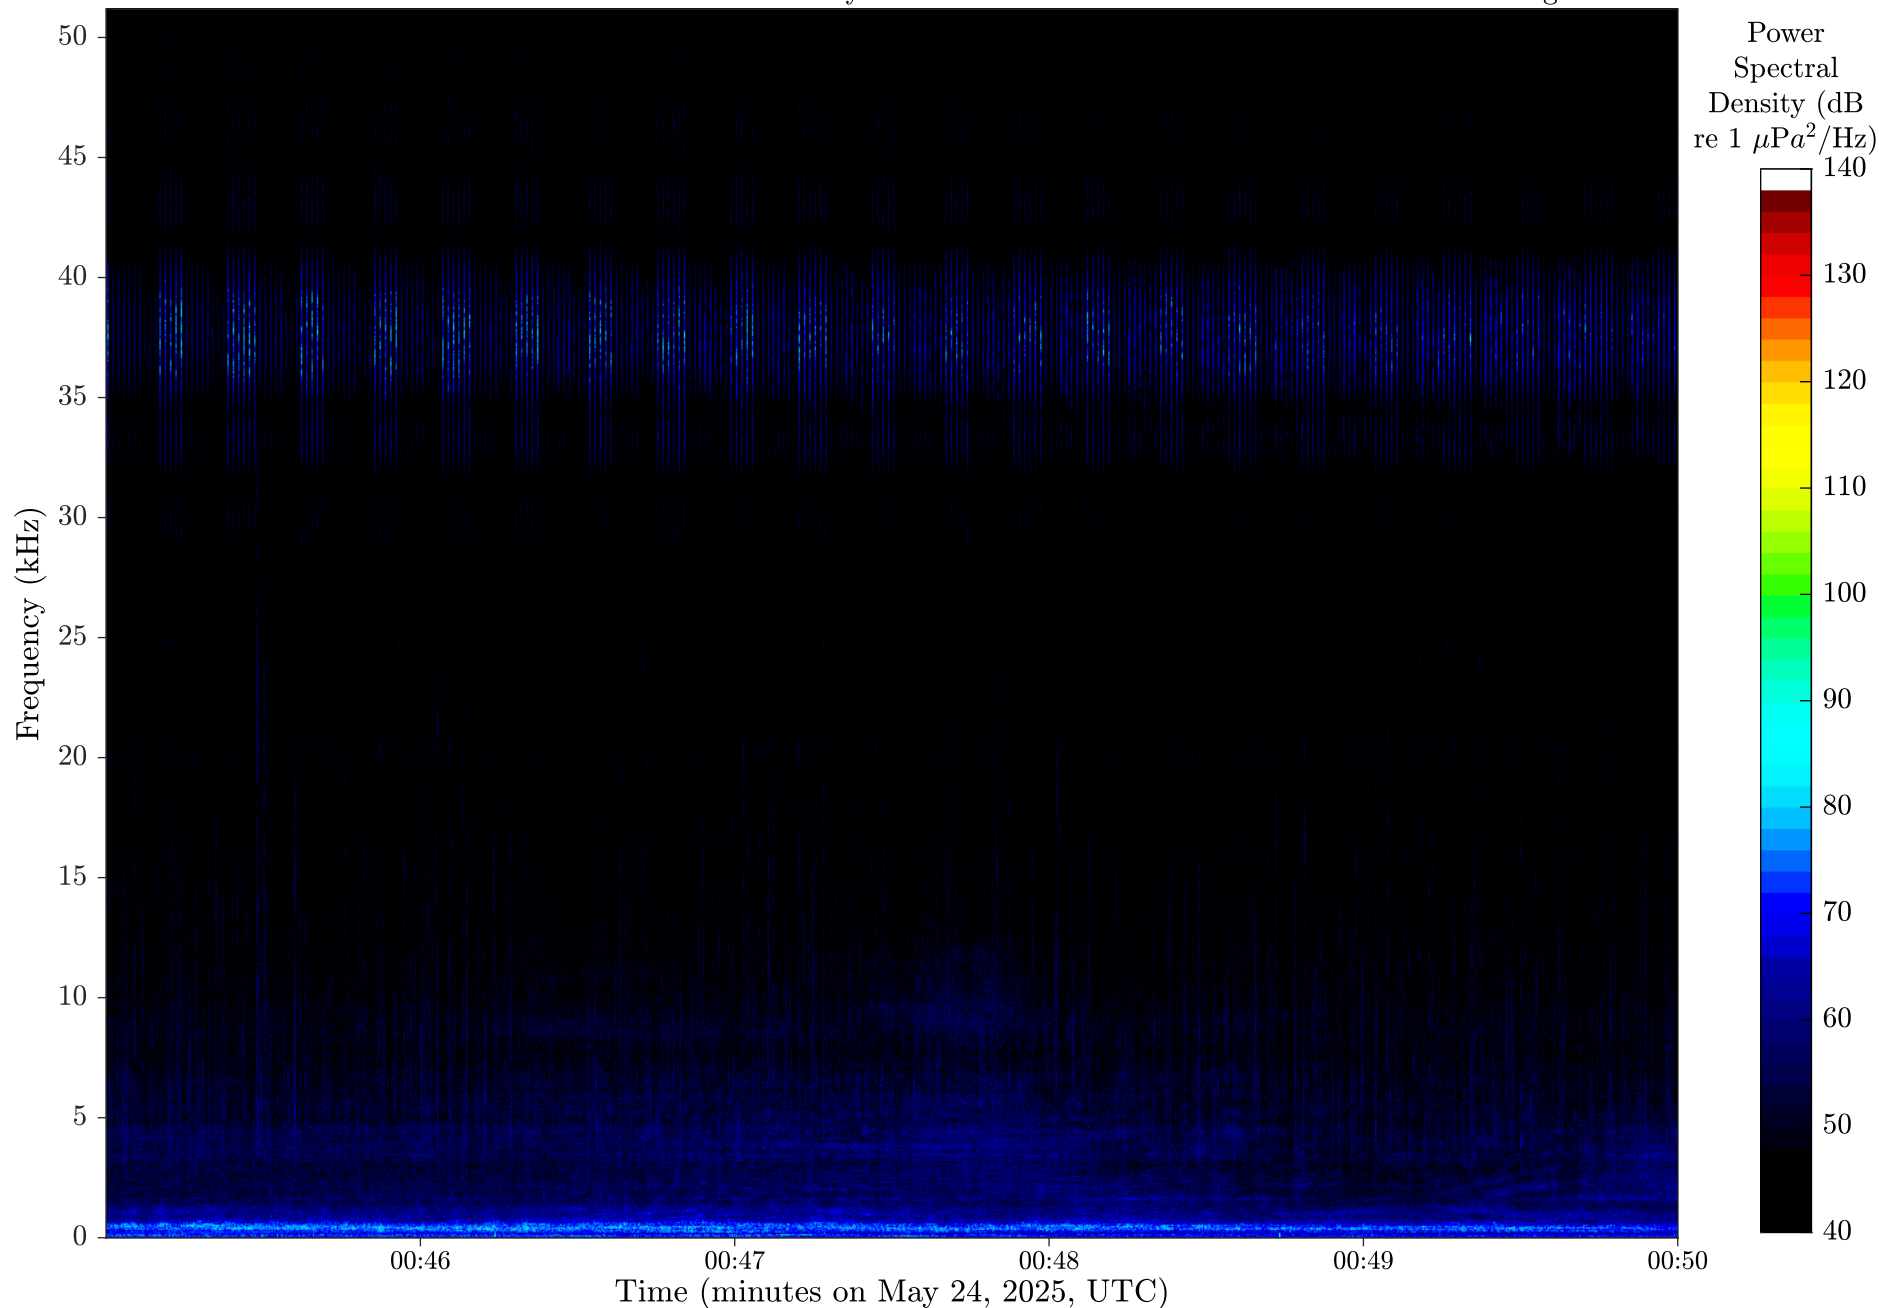


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:09:11 UTC

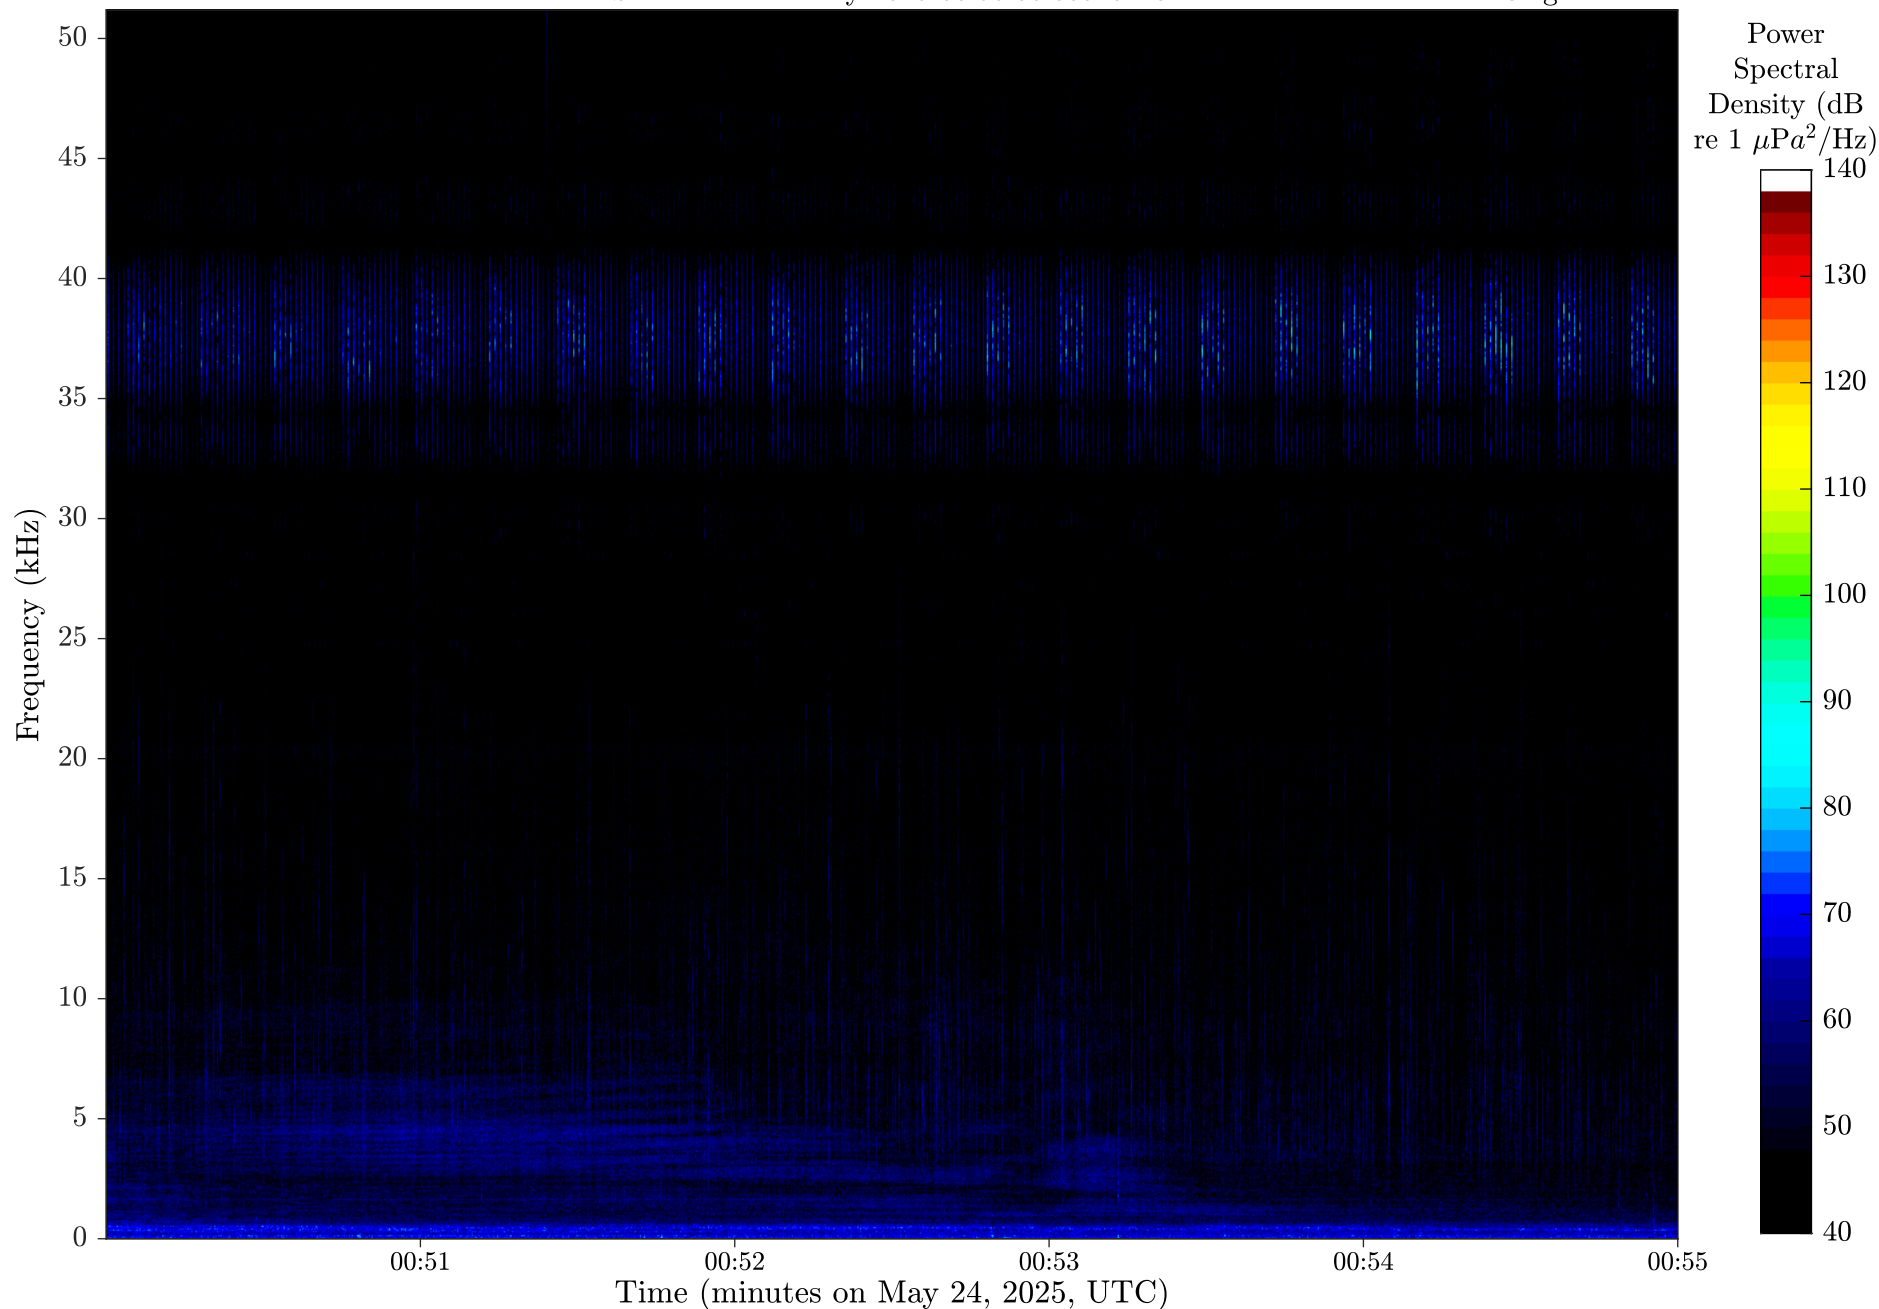


Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:09:19 UTC

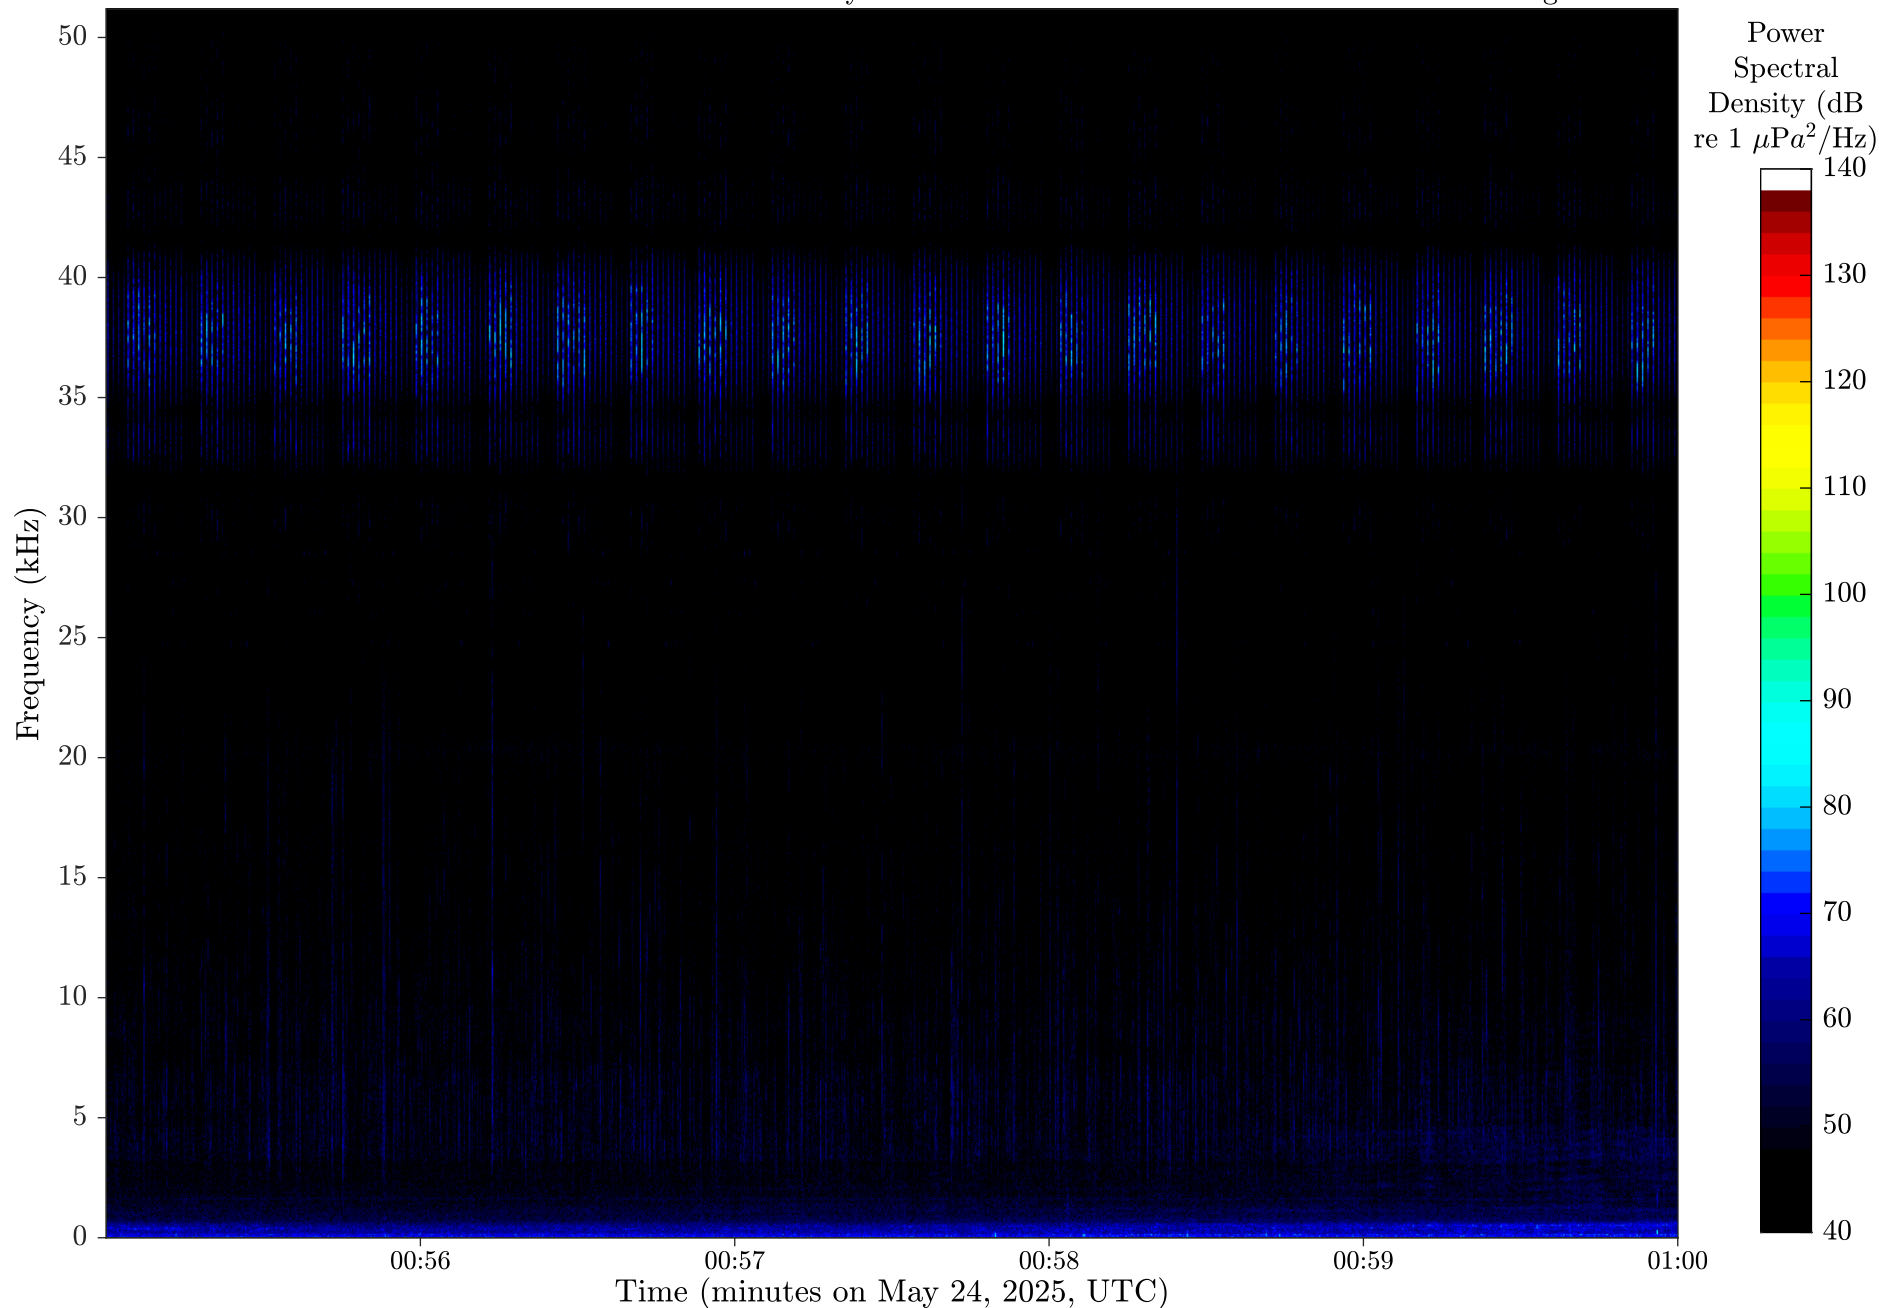


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:09:26 UTC

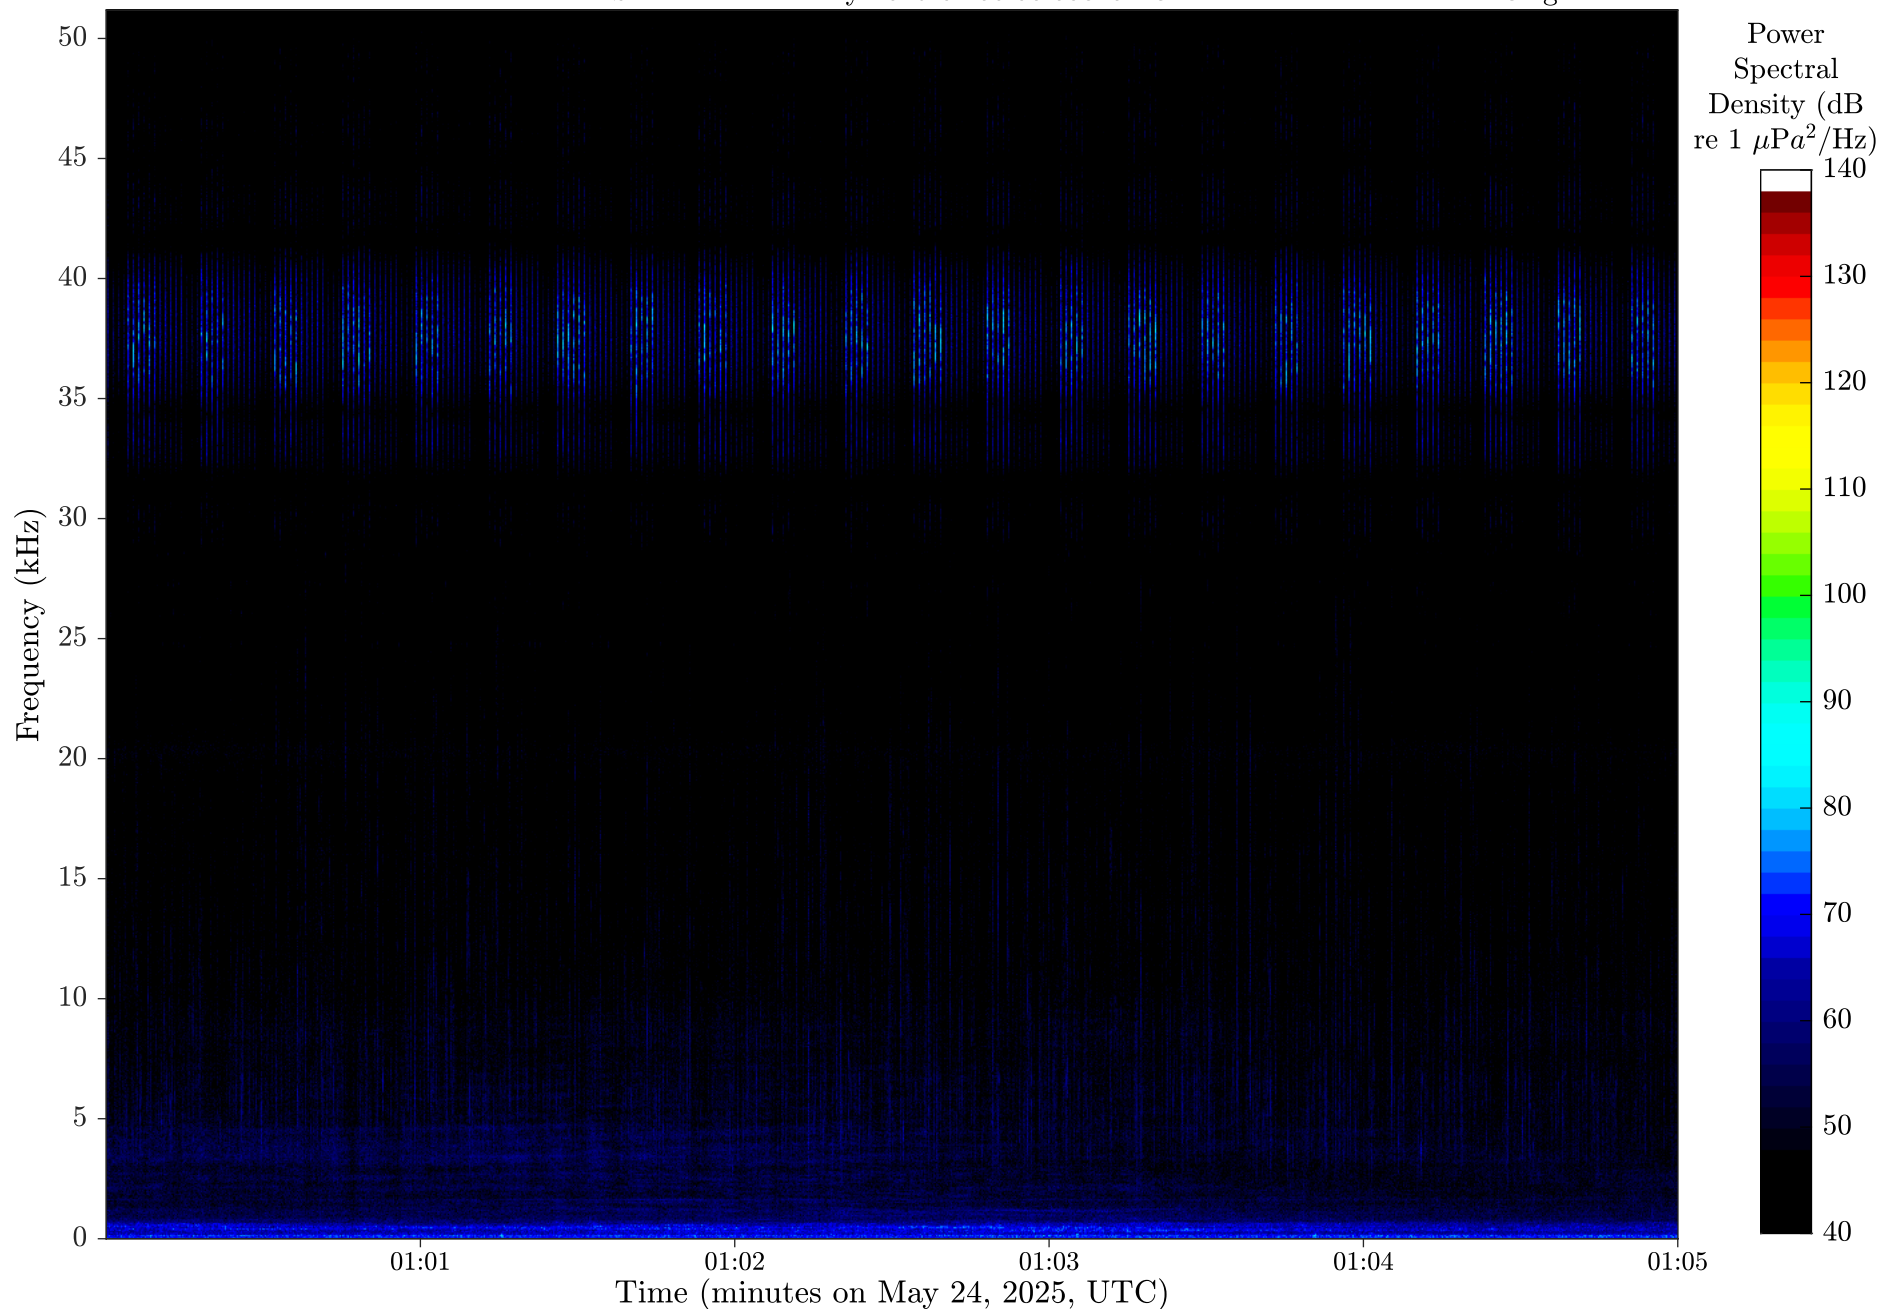


Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:09:34 UTC

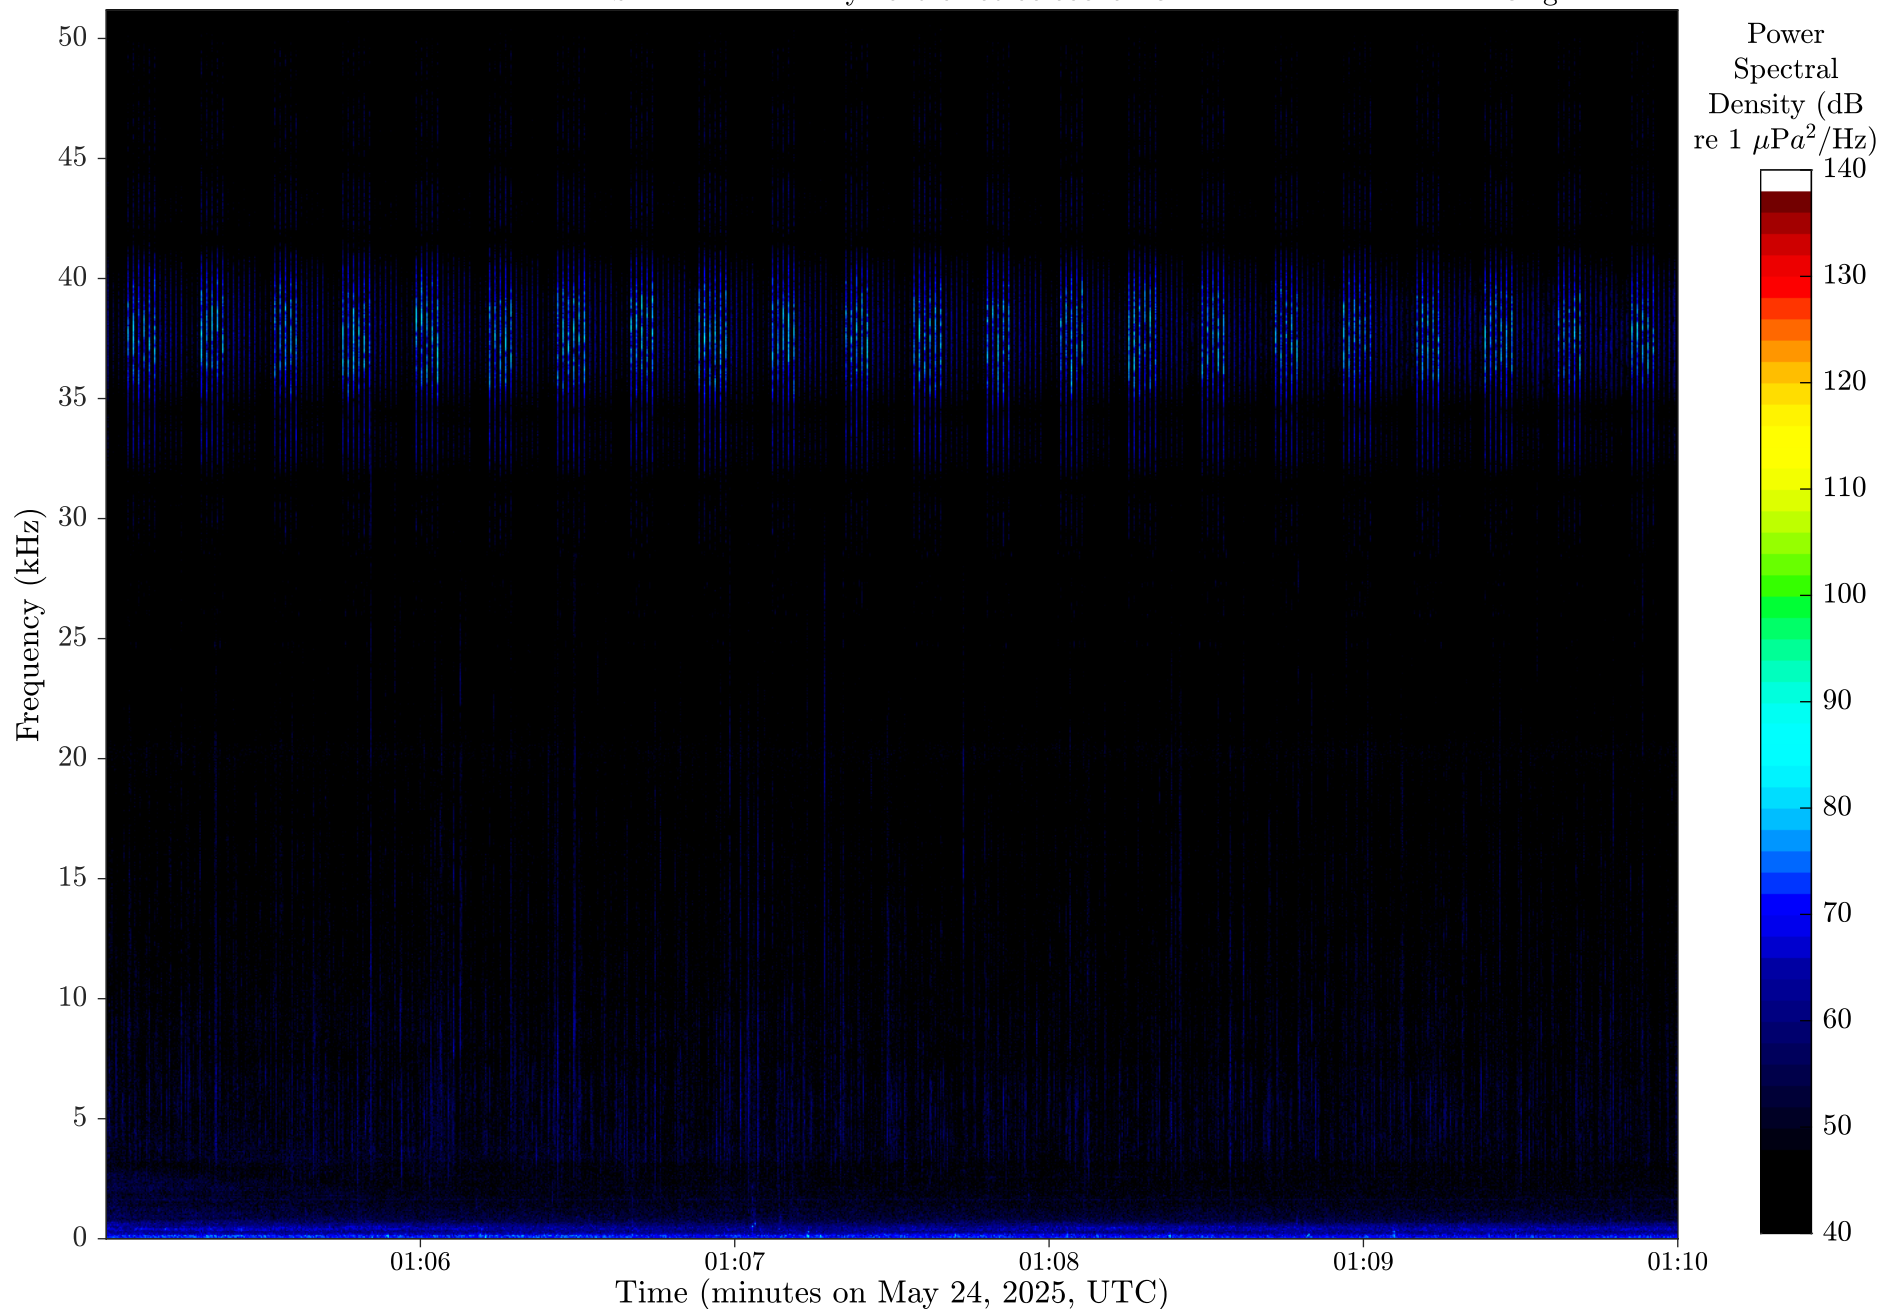


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:09:42 UTC

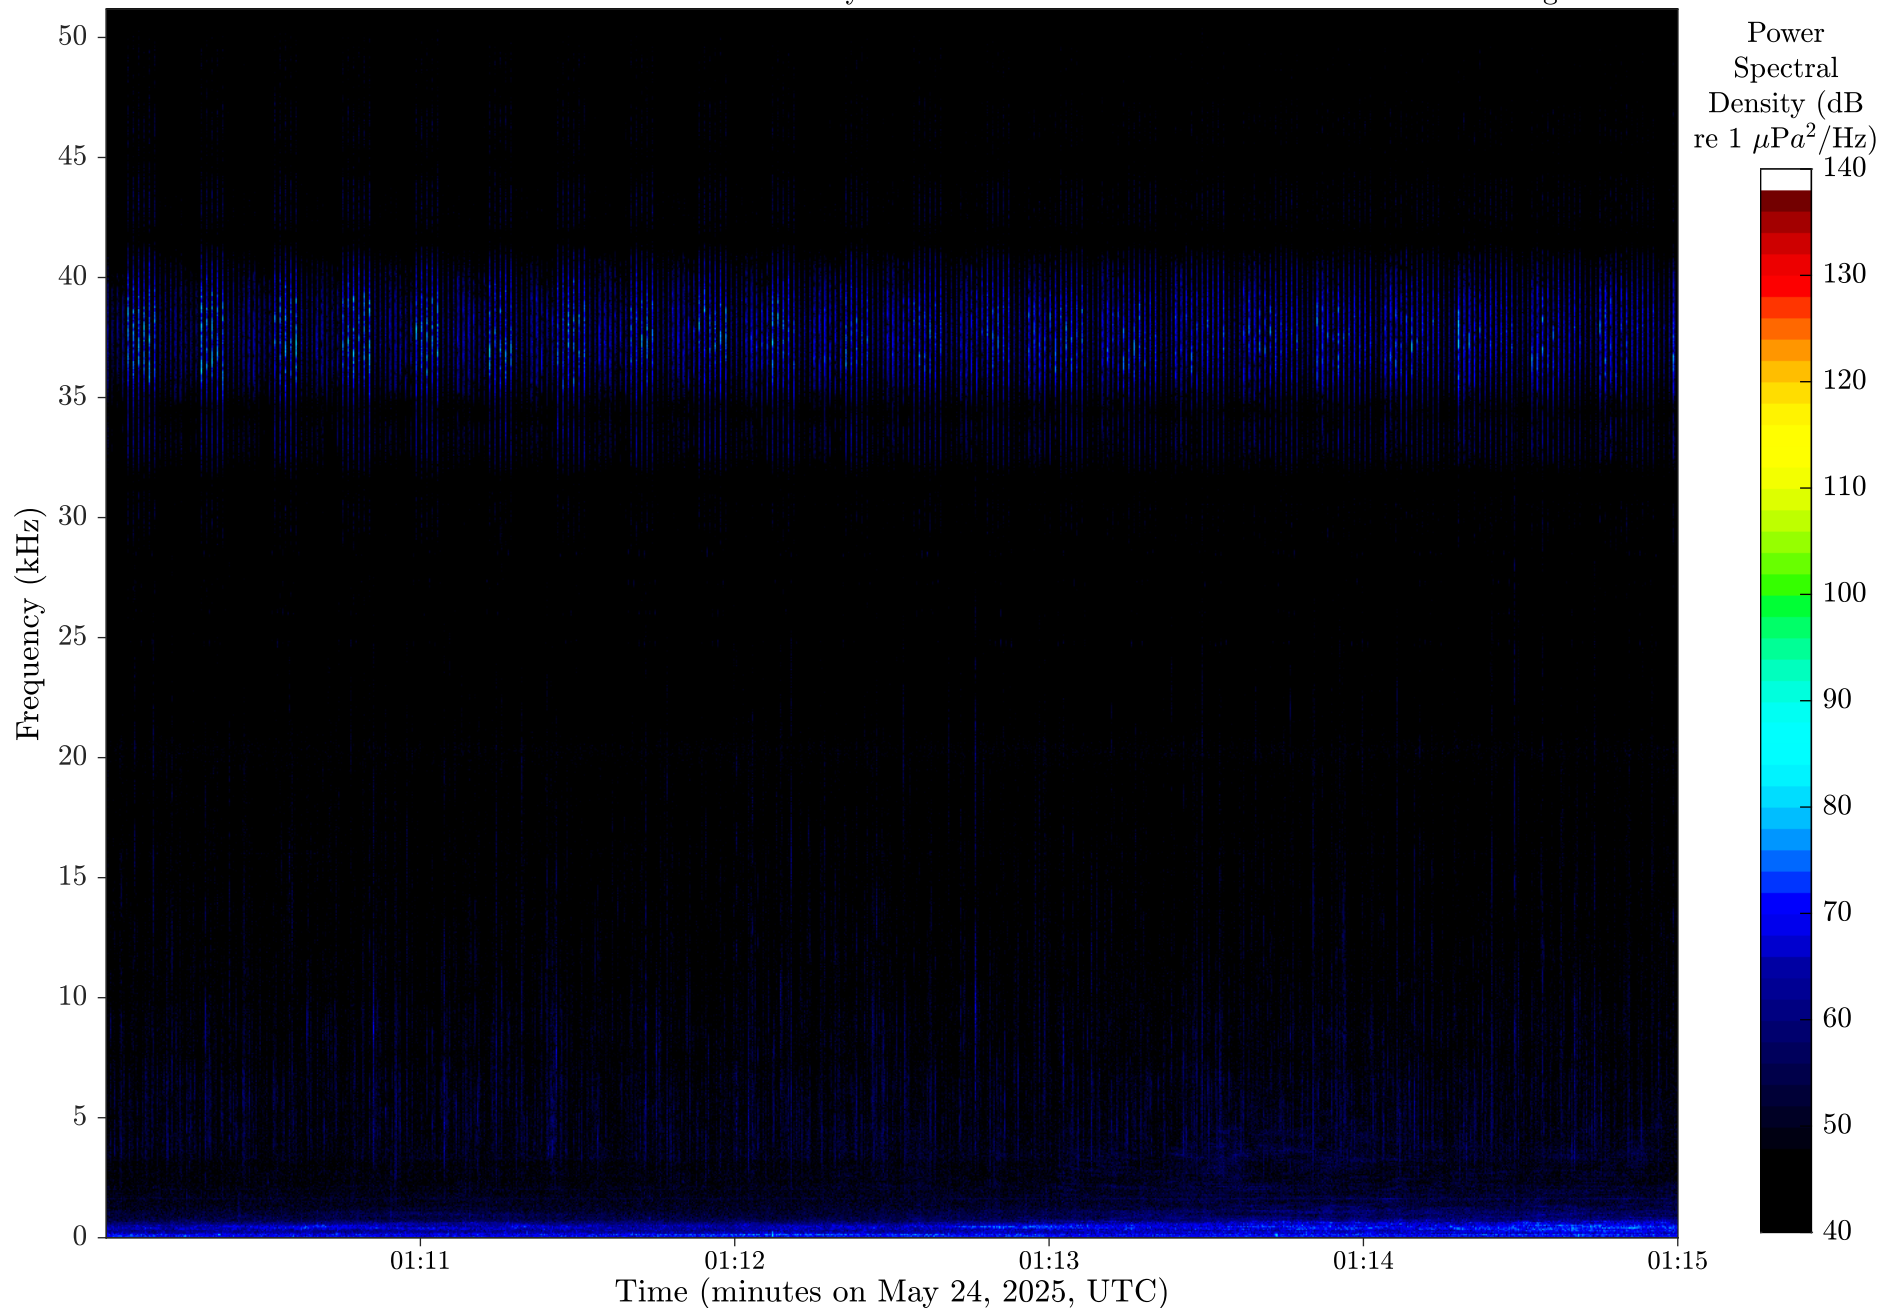


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:09:49 UTC

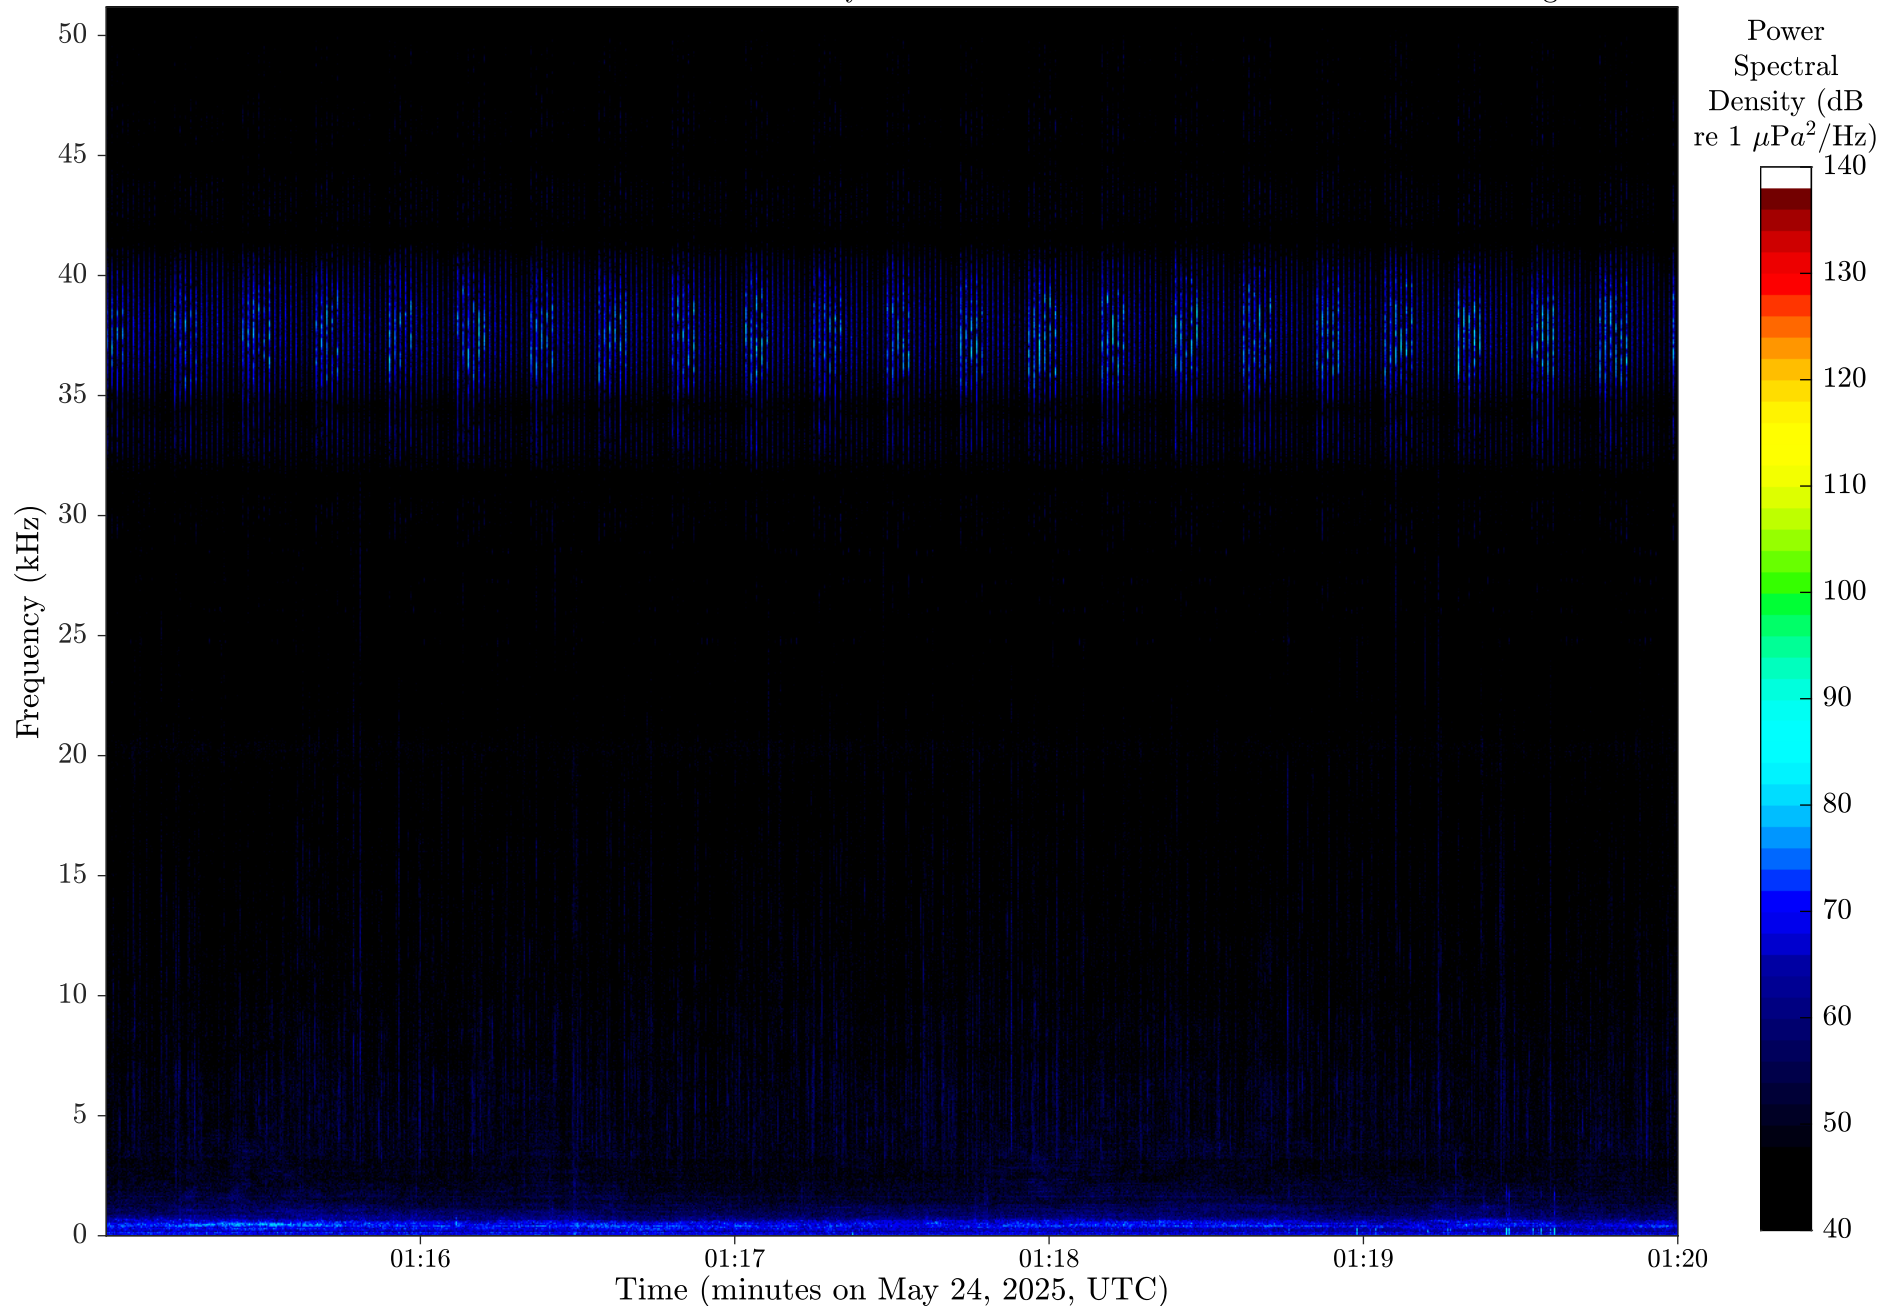


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:09:56 UTC

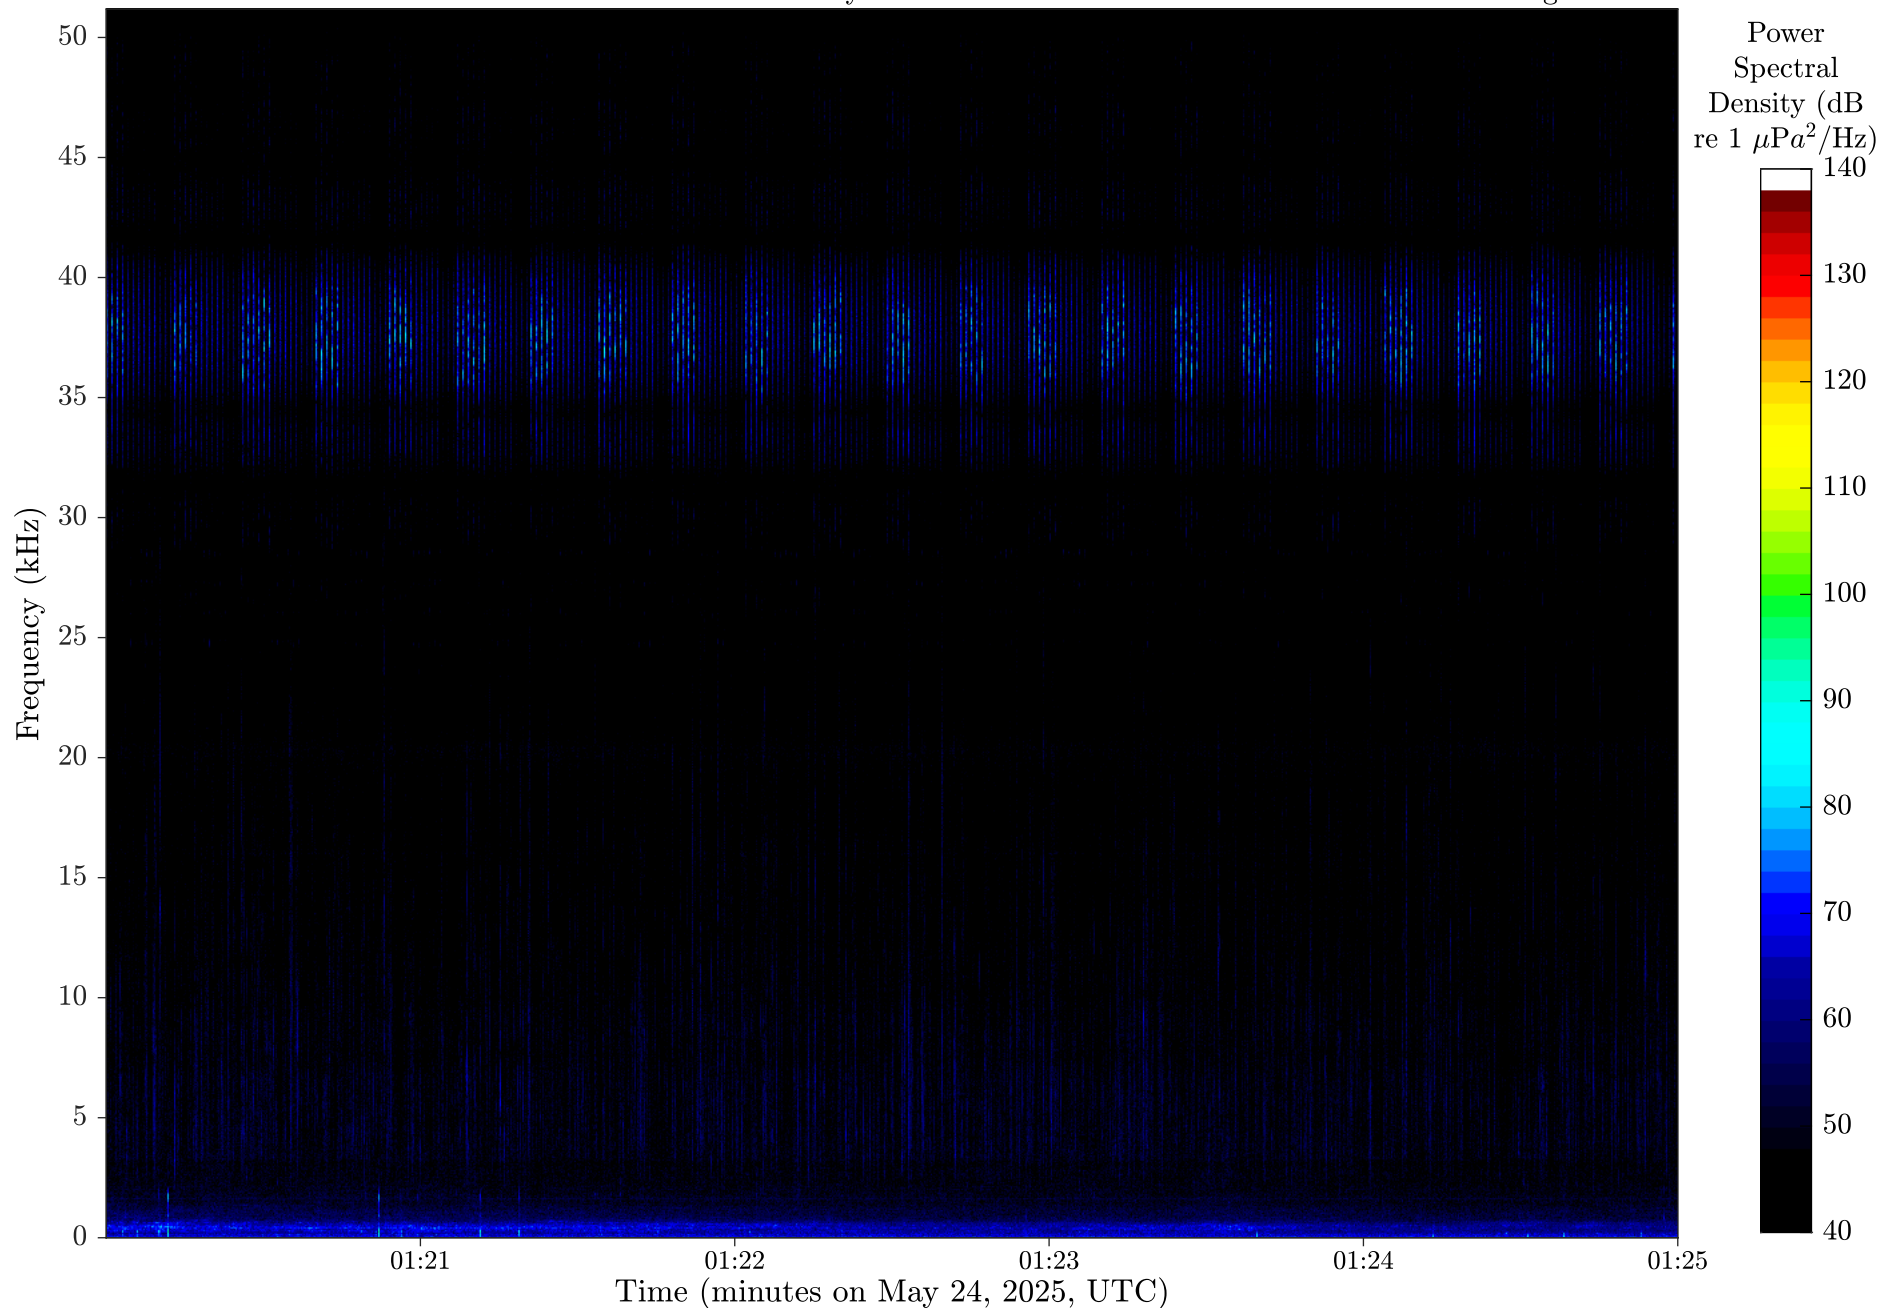


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:10:04 UTC

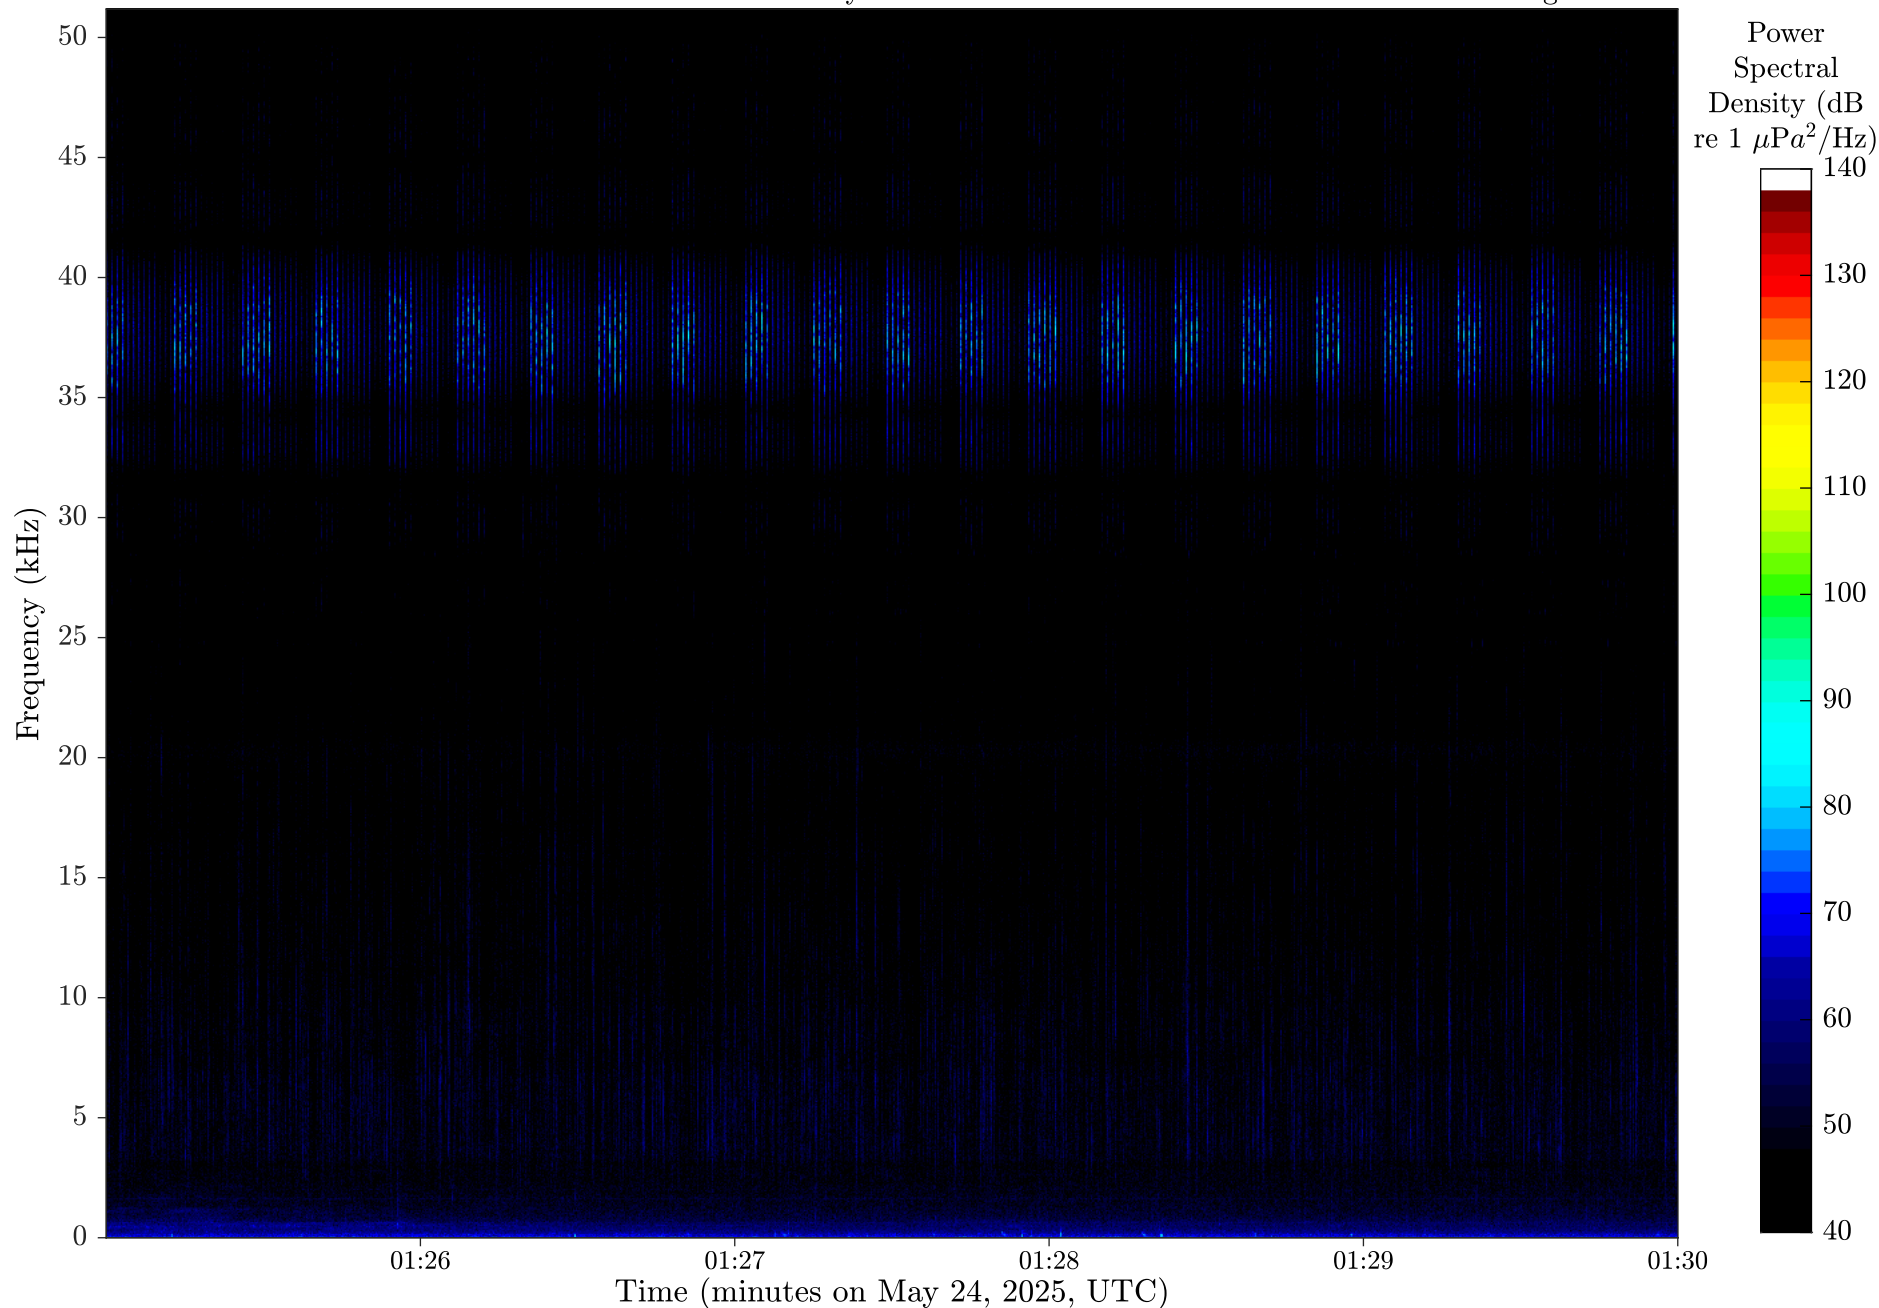


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:10:11 UTC

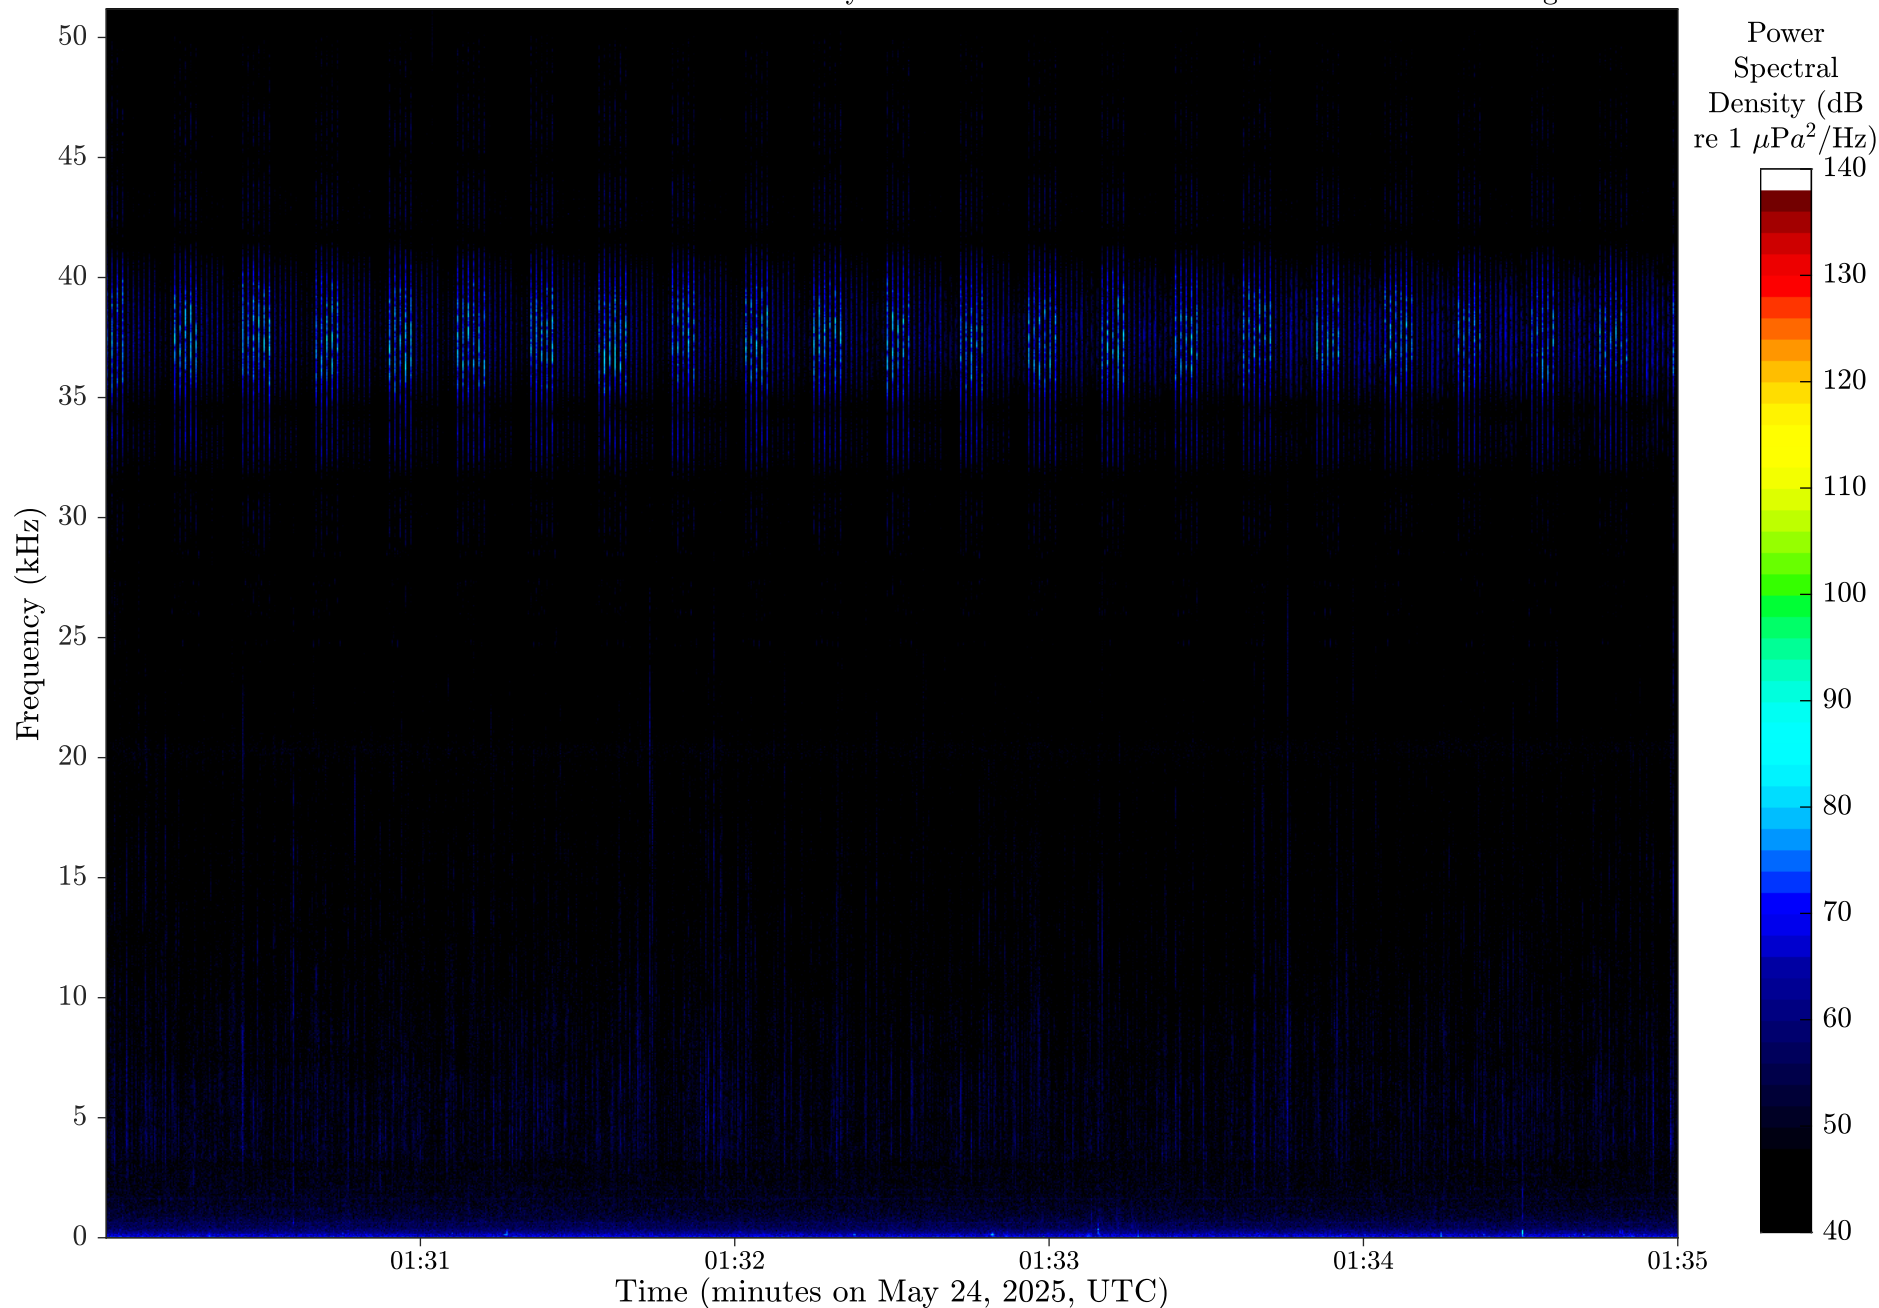


Comments: 34.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:10:19 UTC

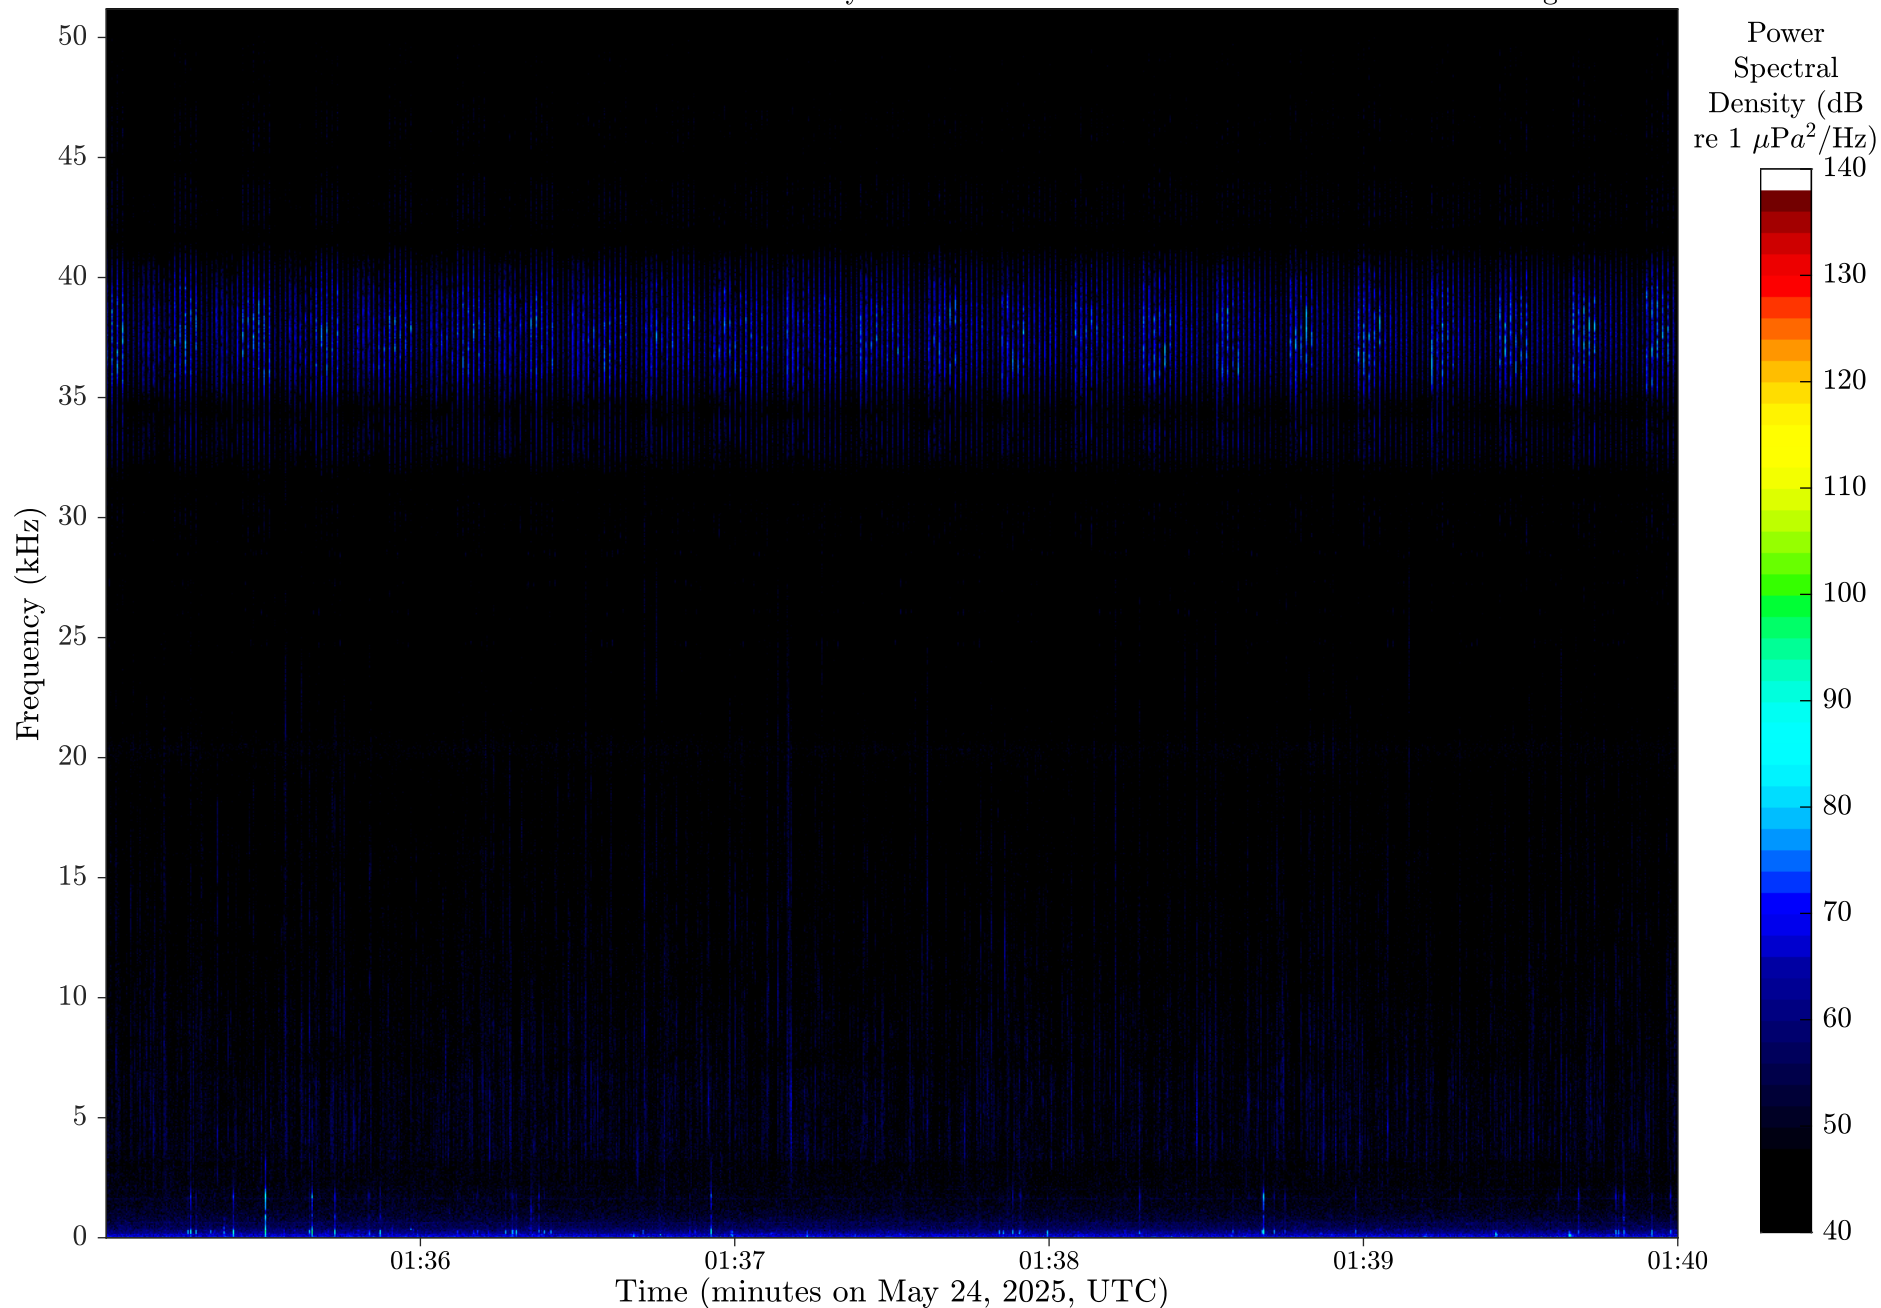


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:10:27 UTC

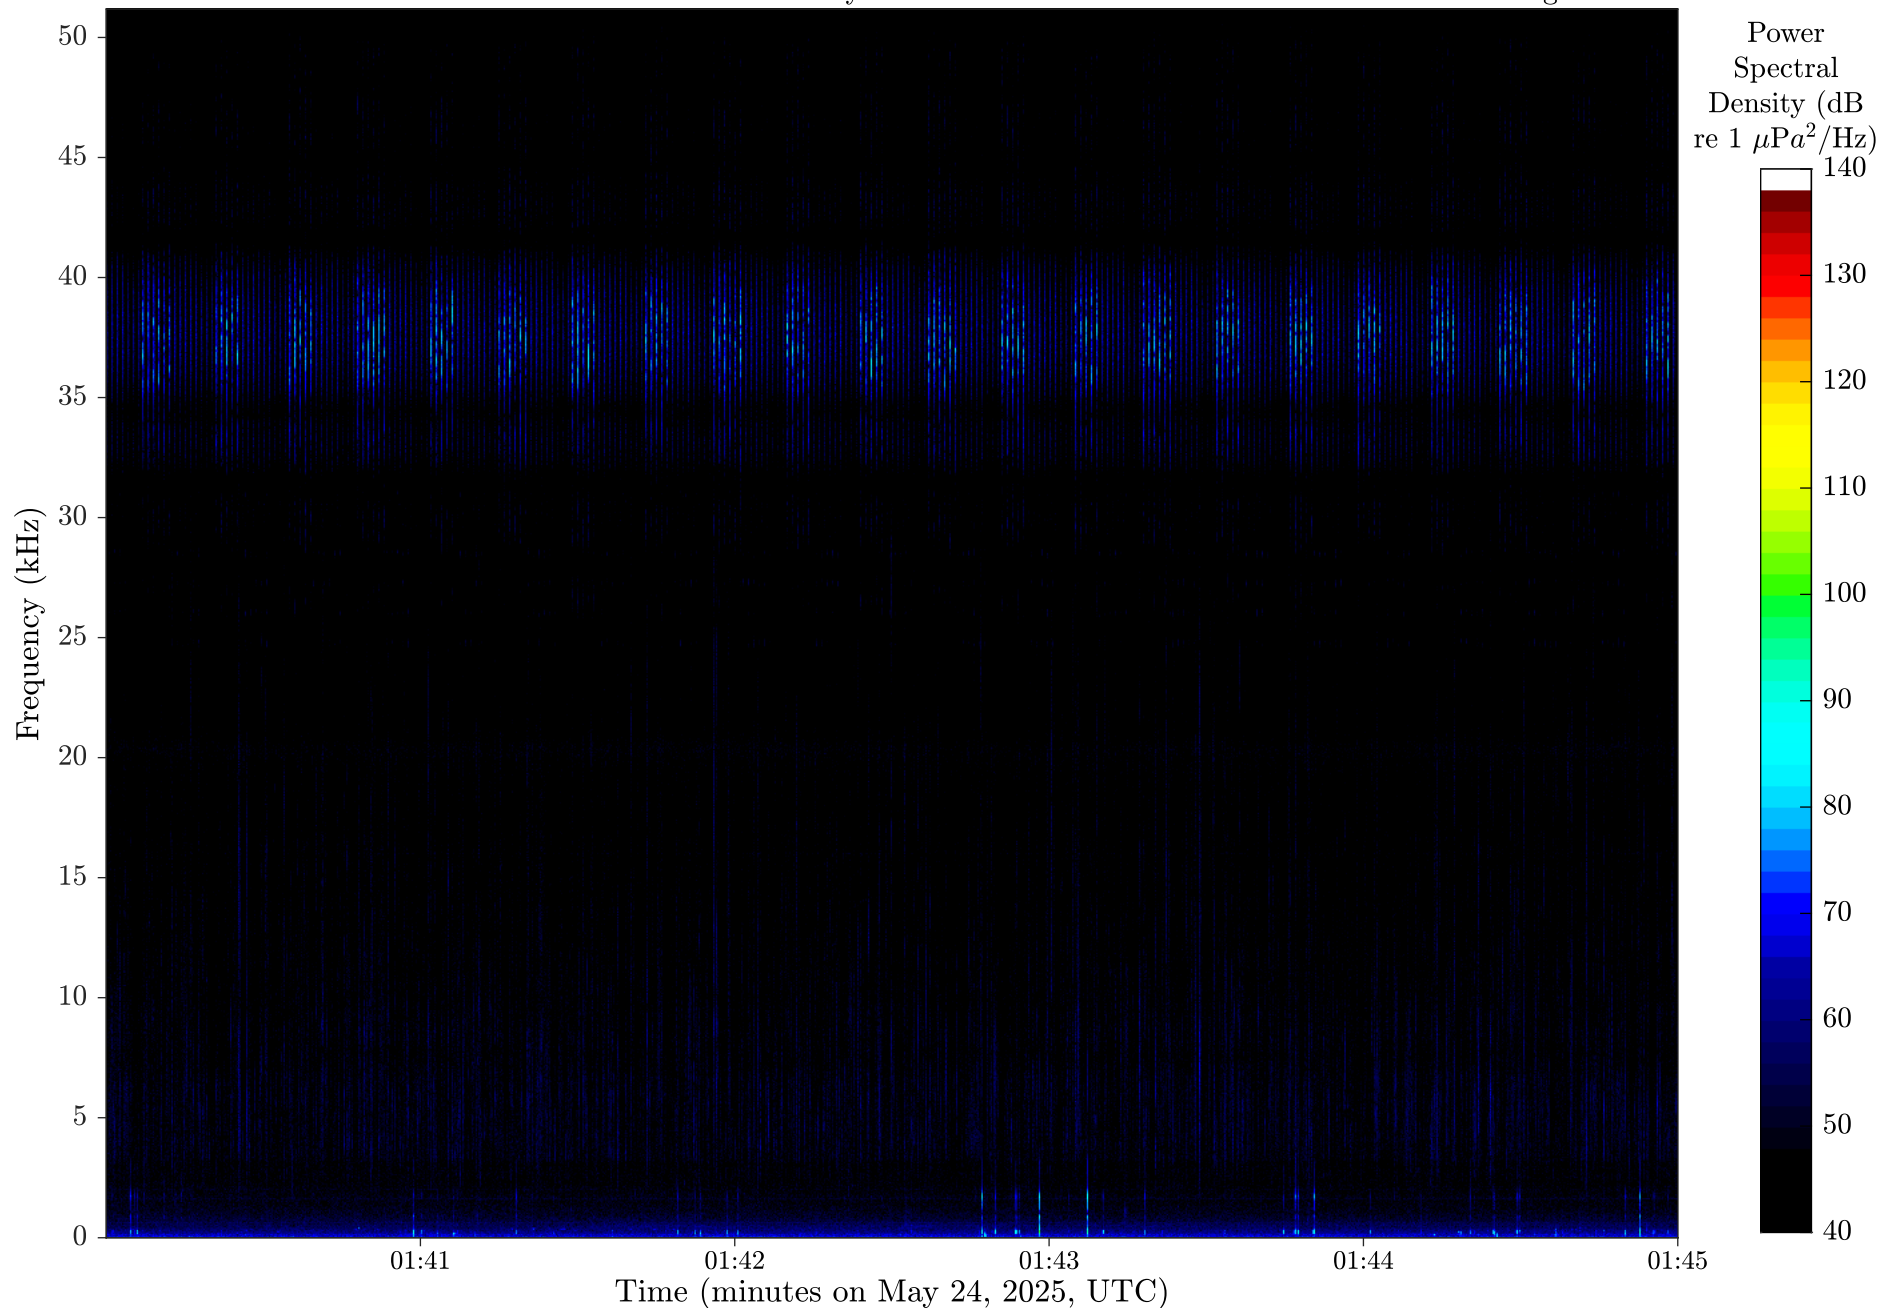


Comments: 34.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:10:34 UTC

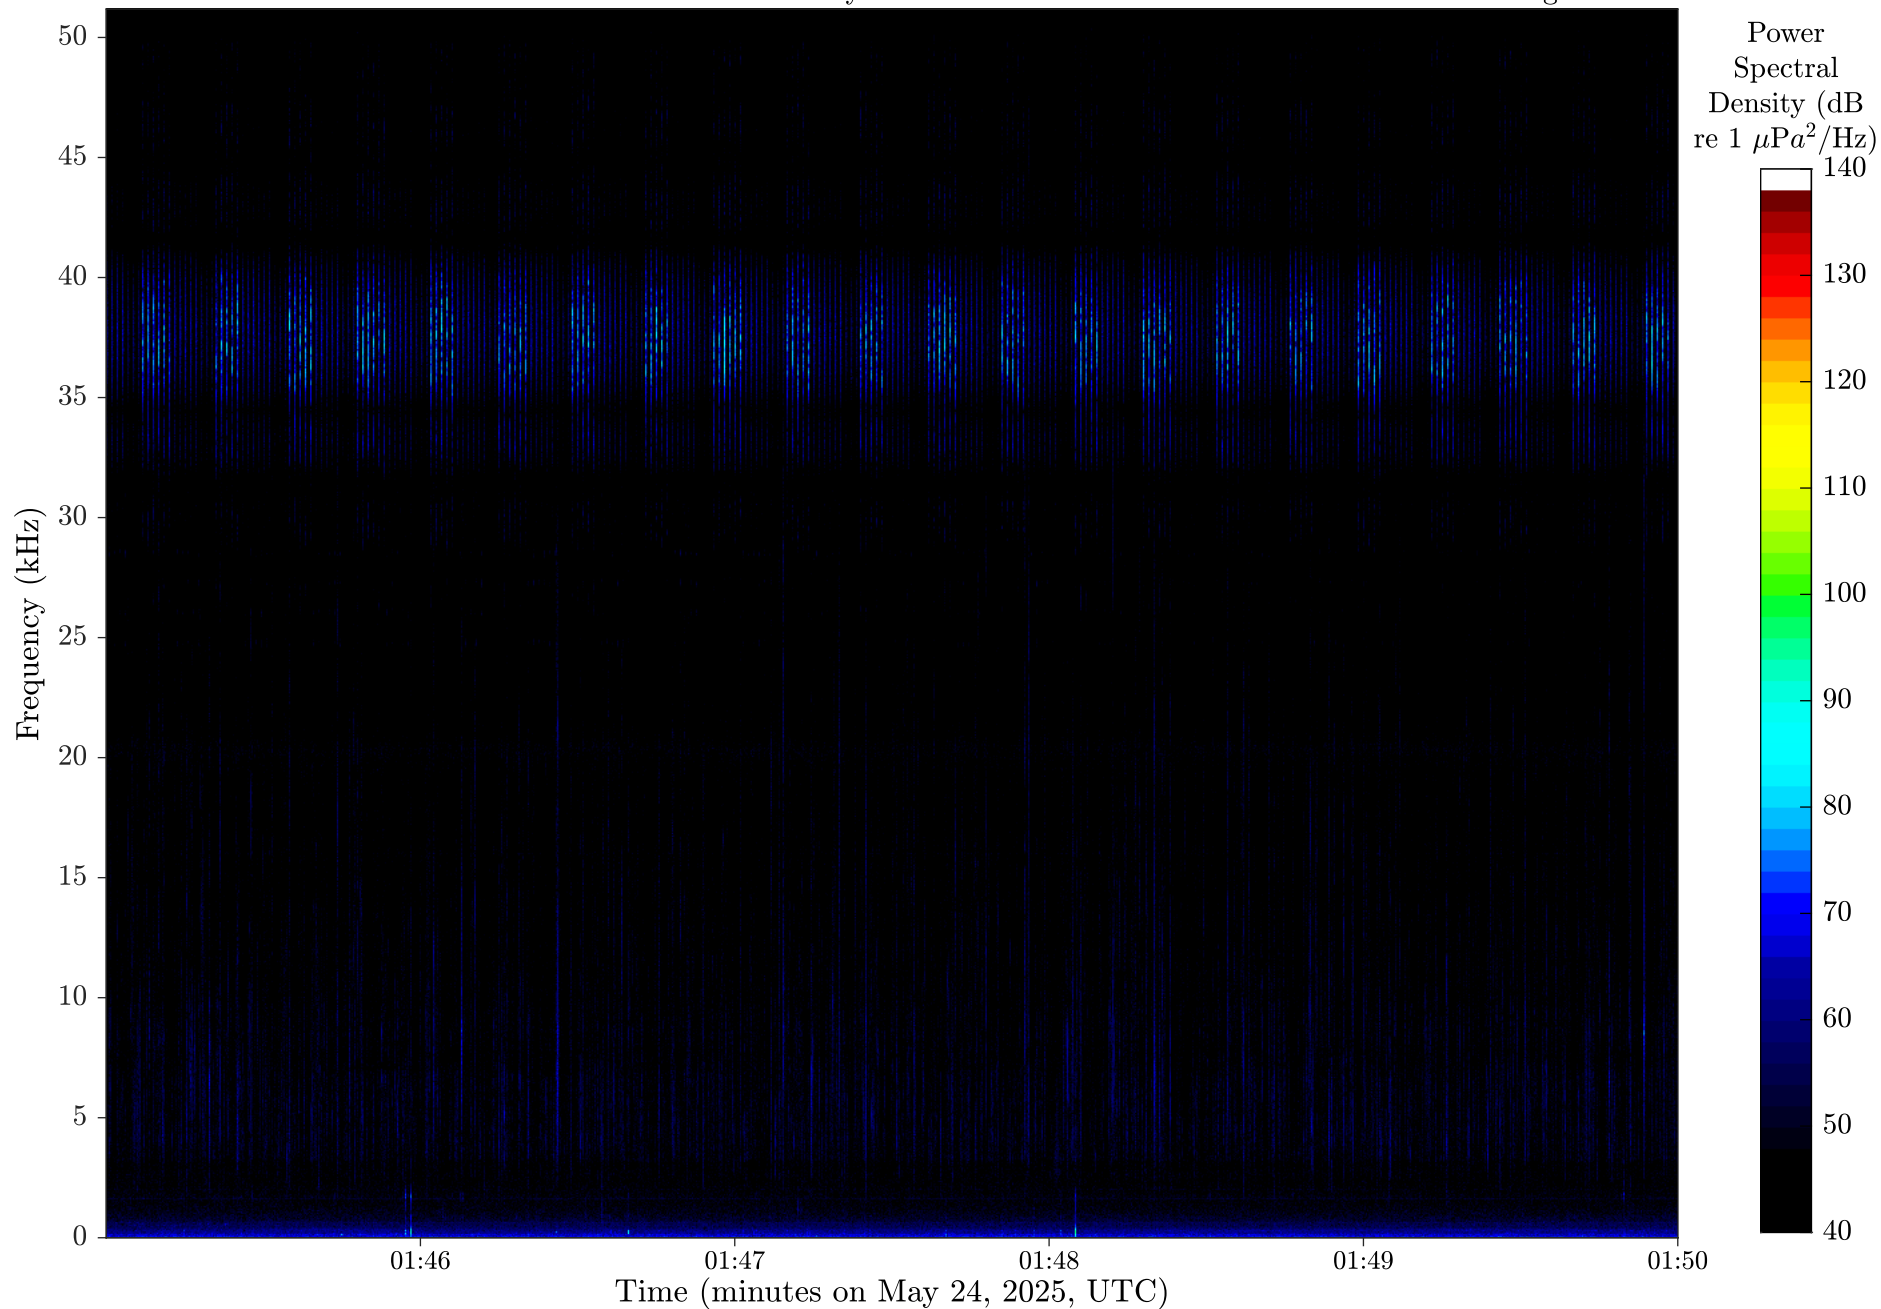


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:10:41 UTC

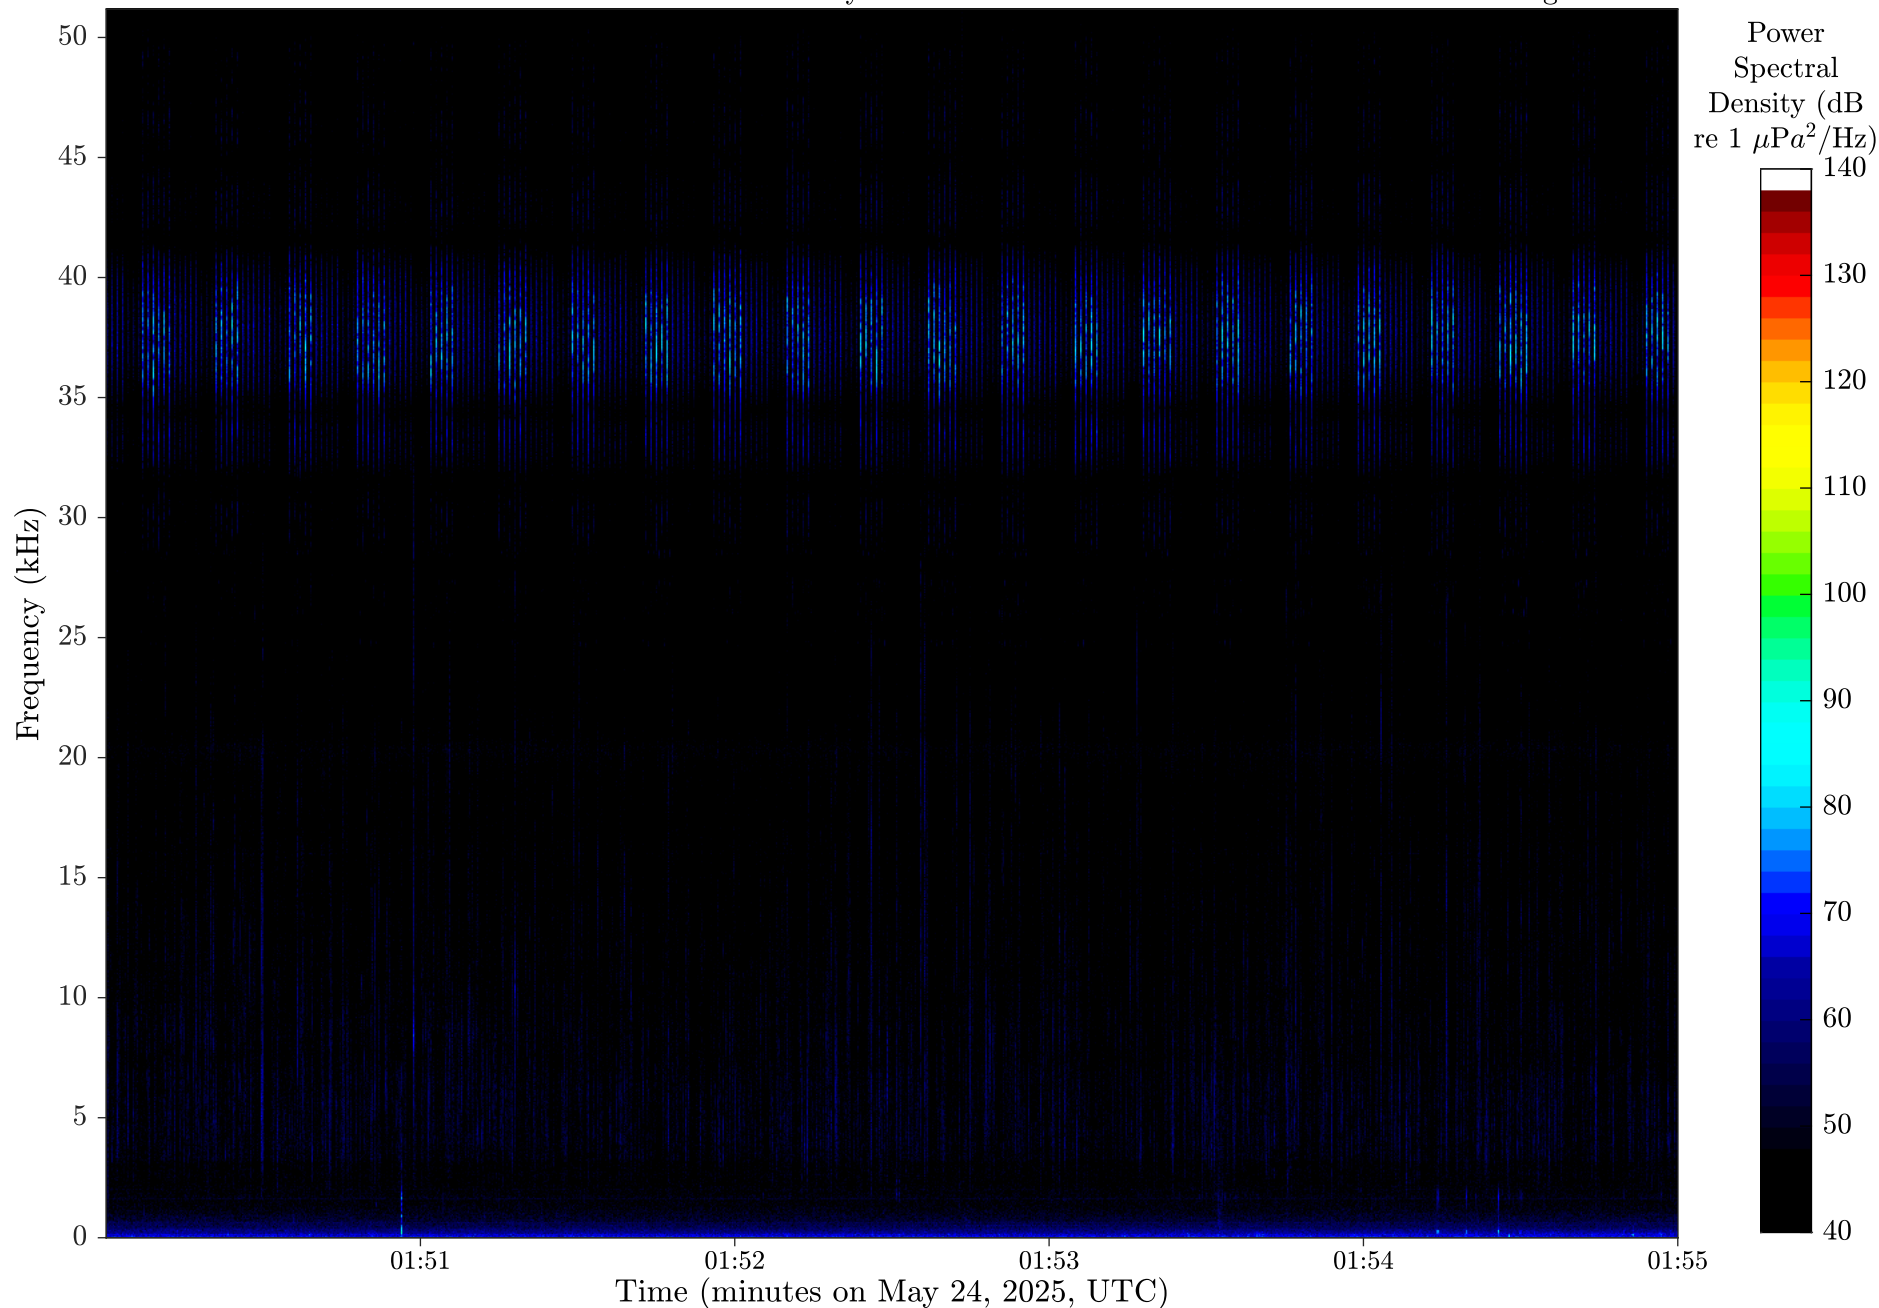


Comments: 36.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:10:49 UTC

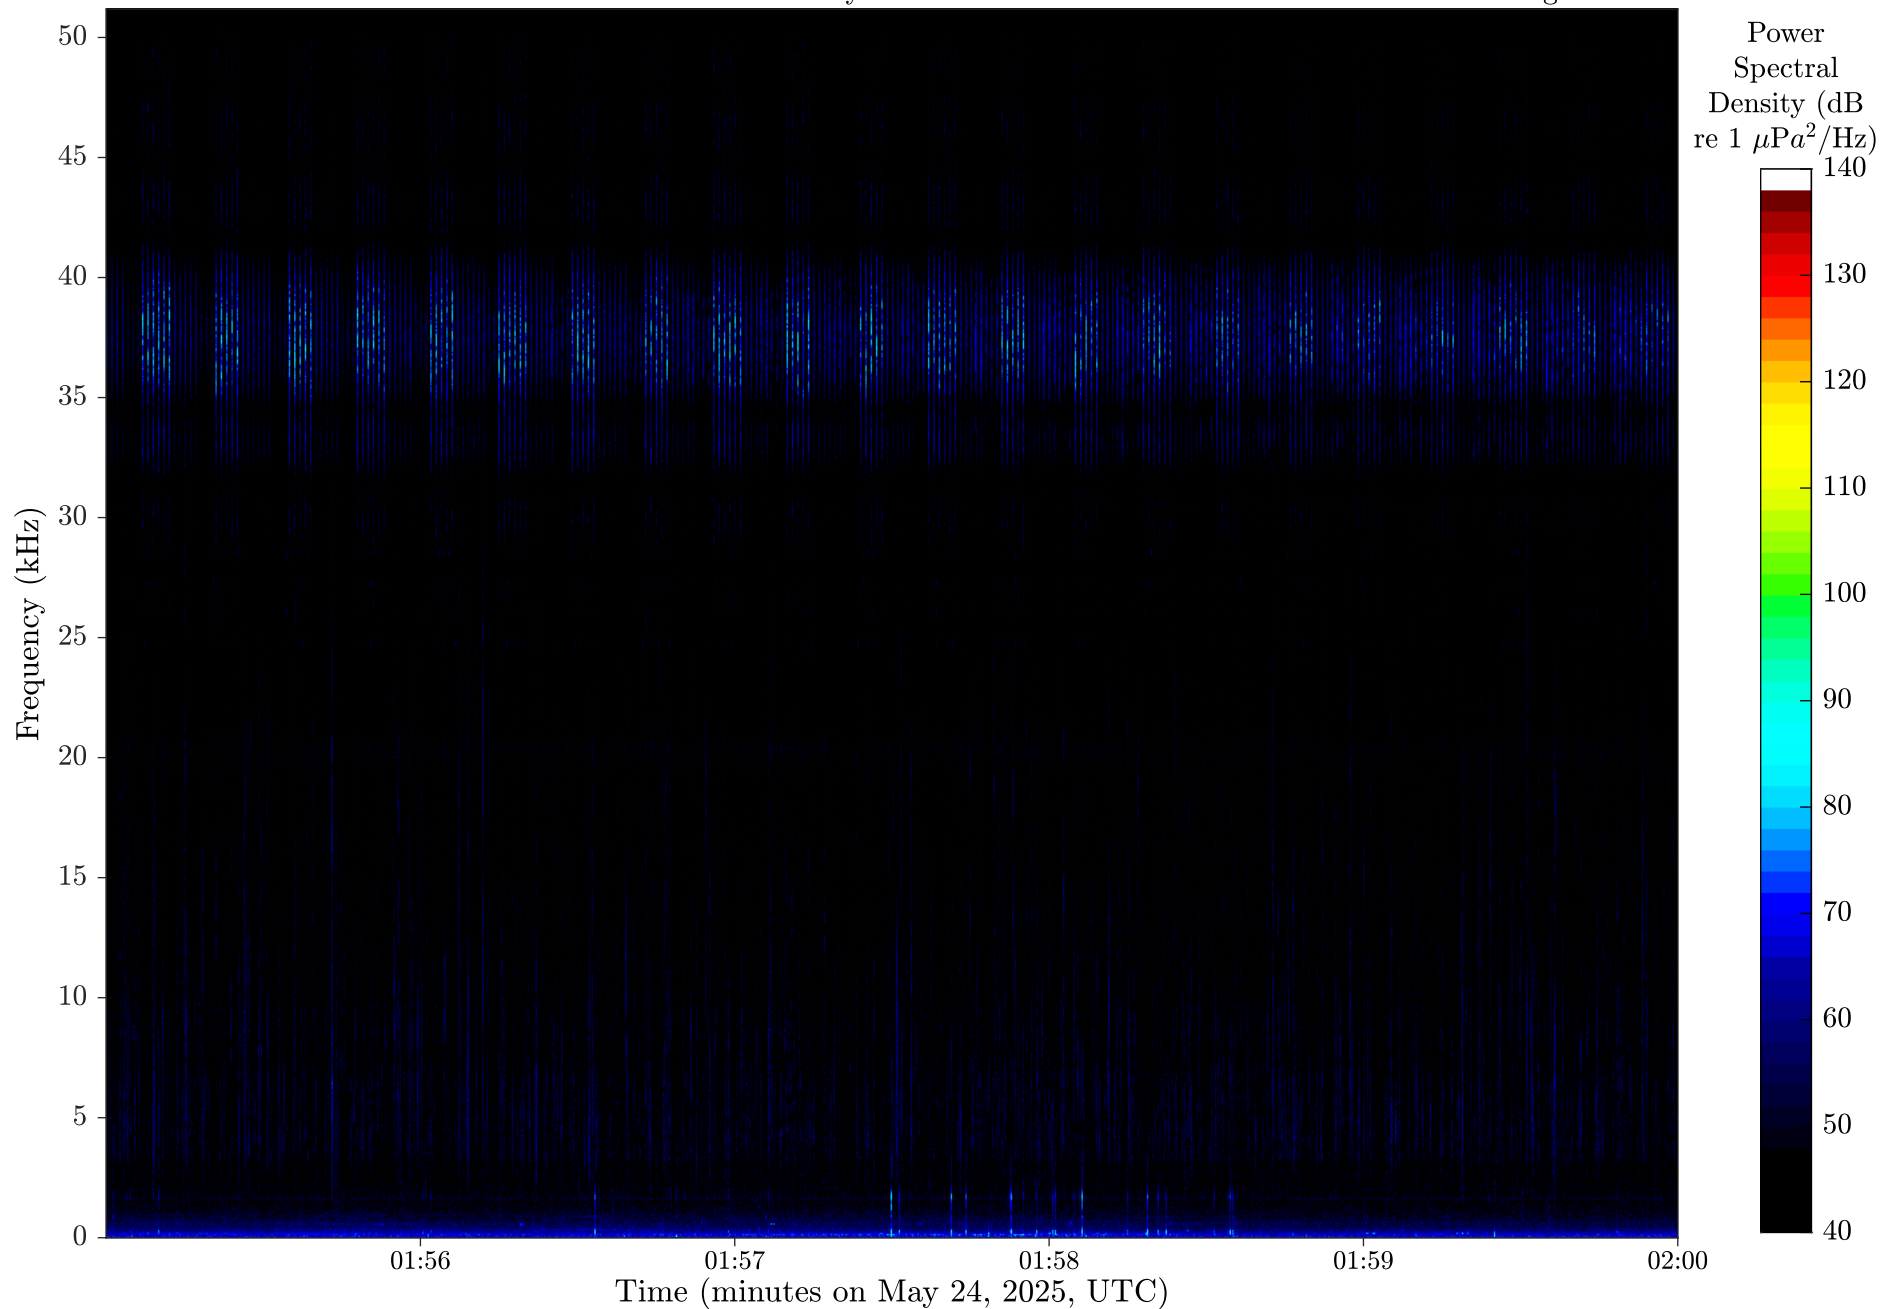


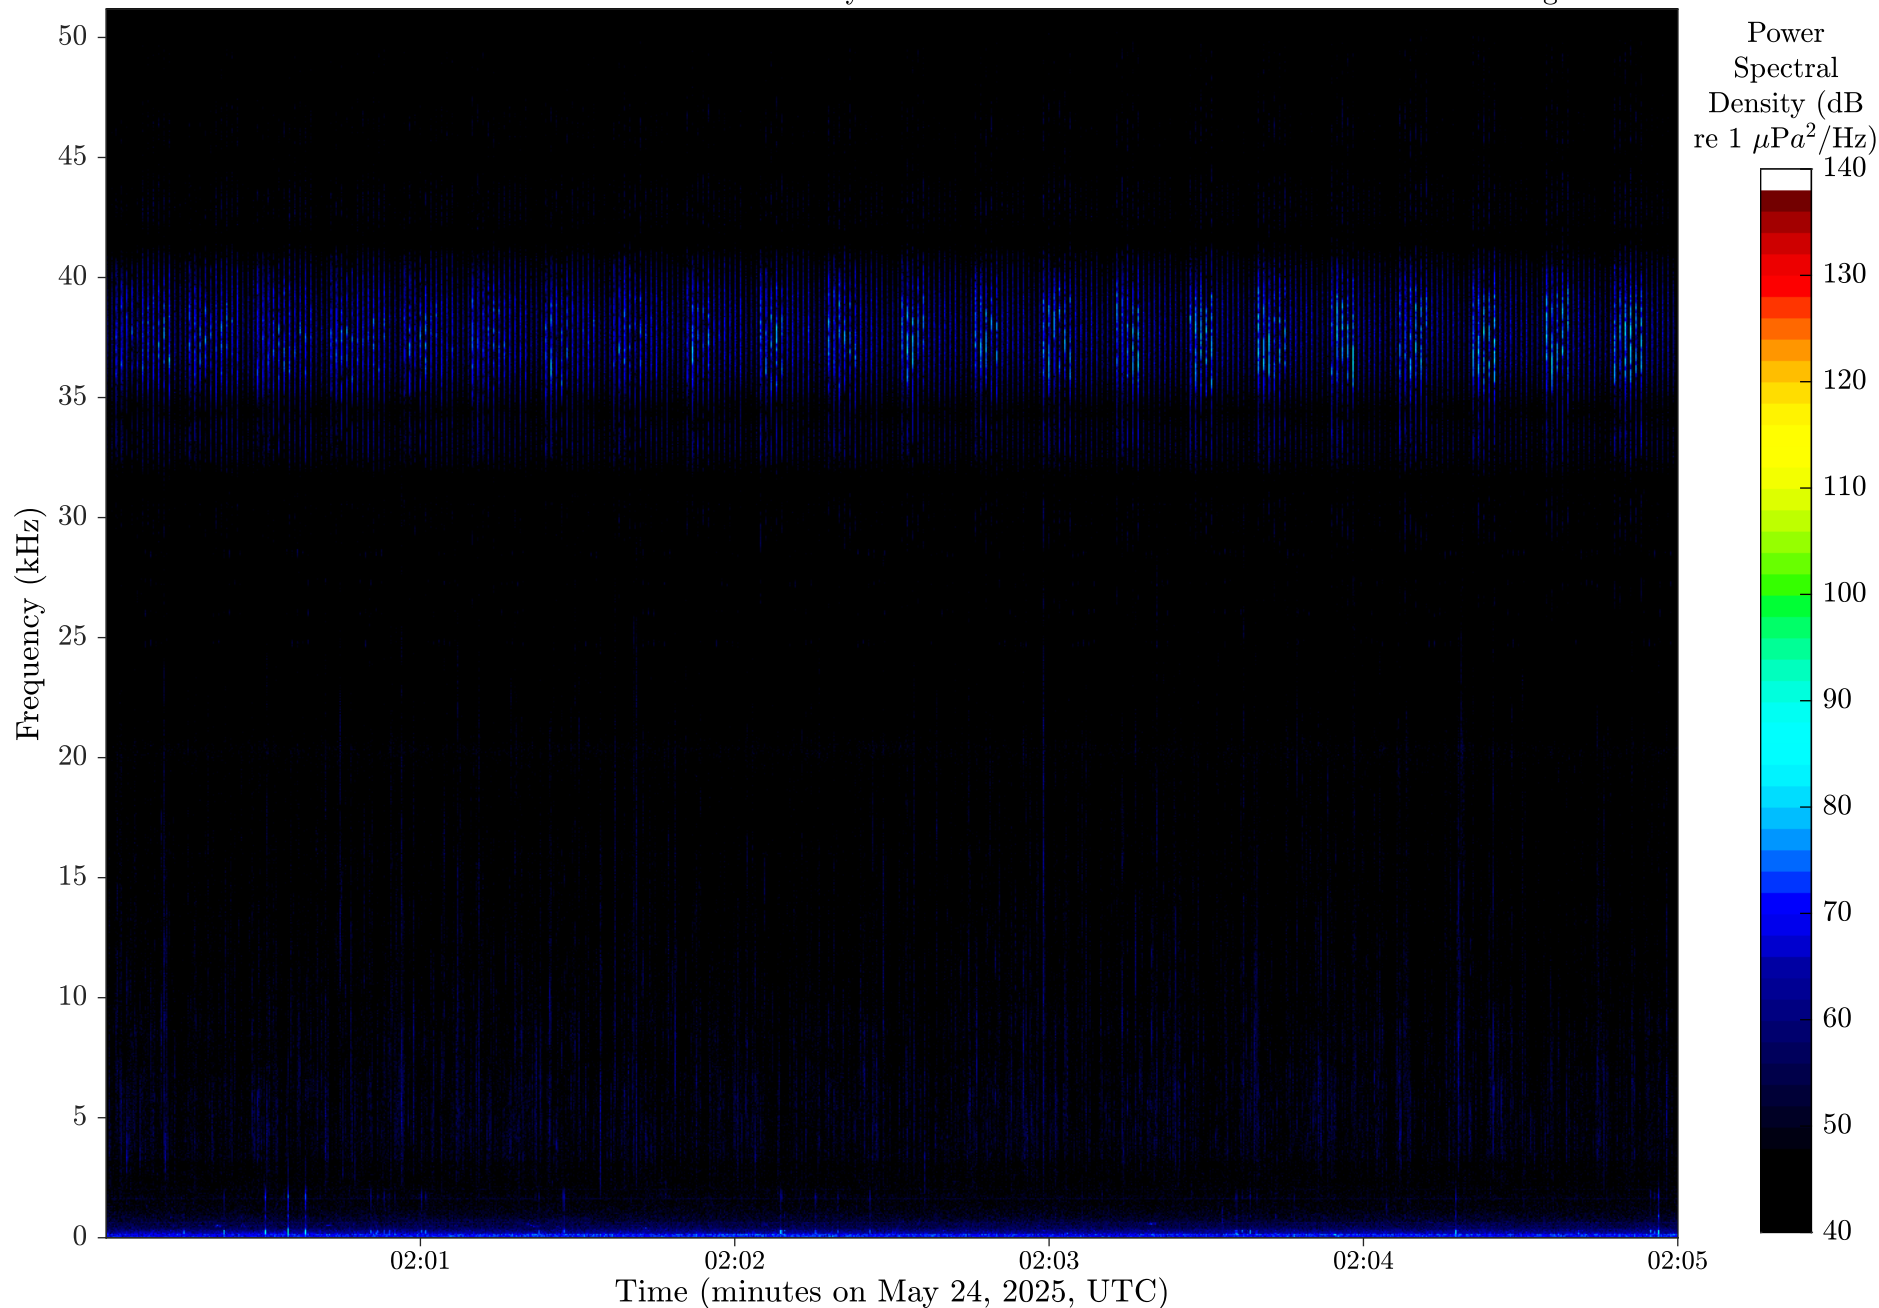

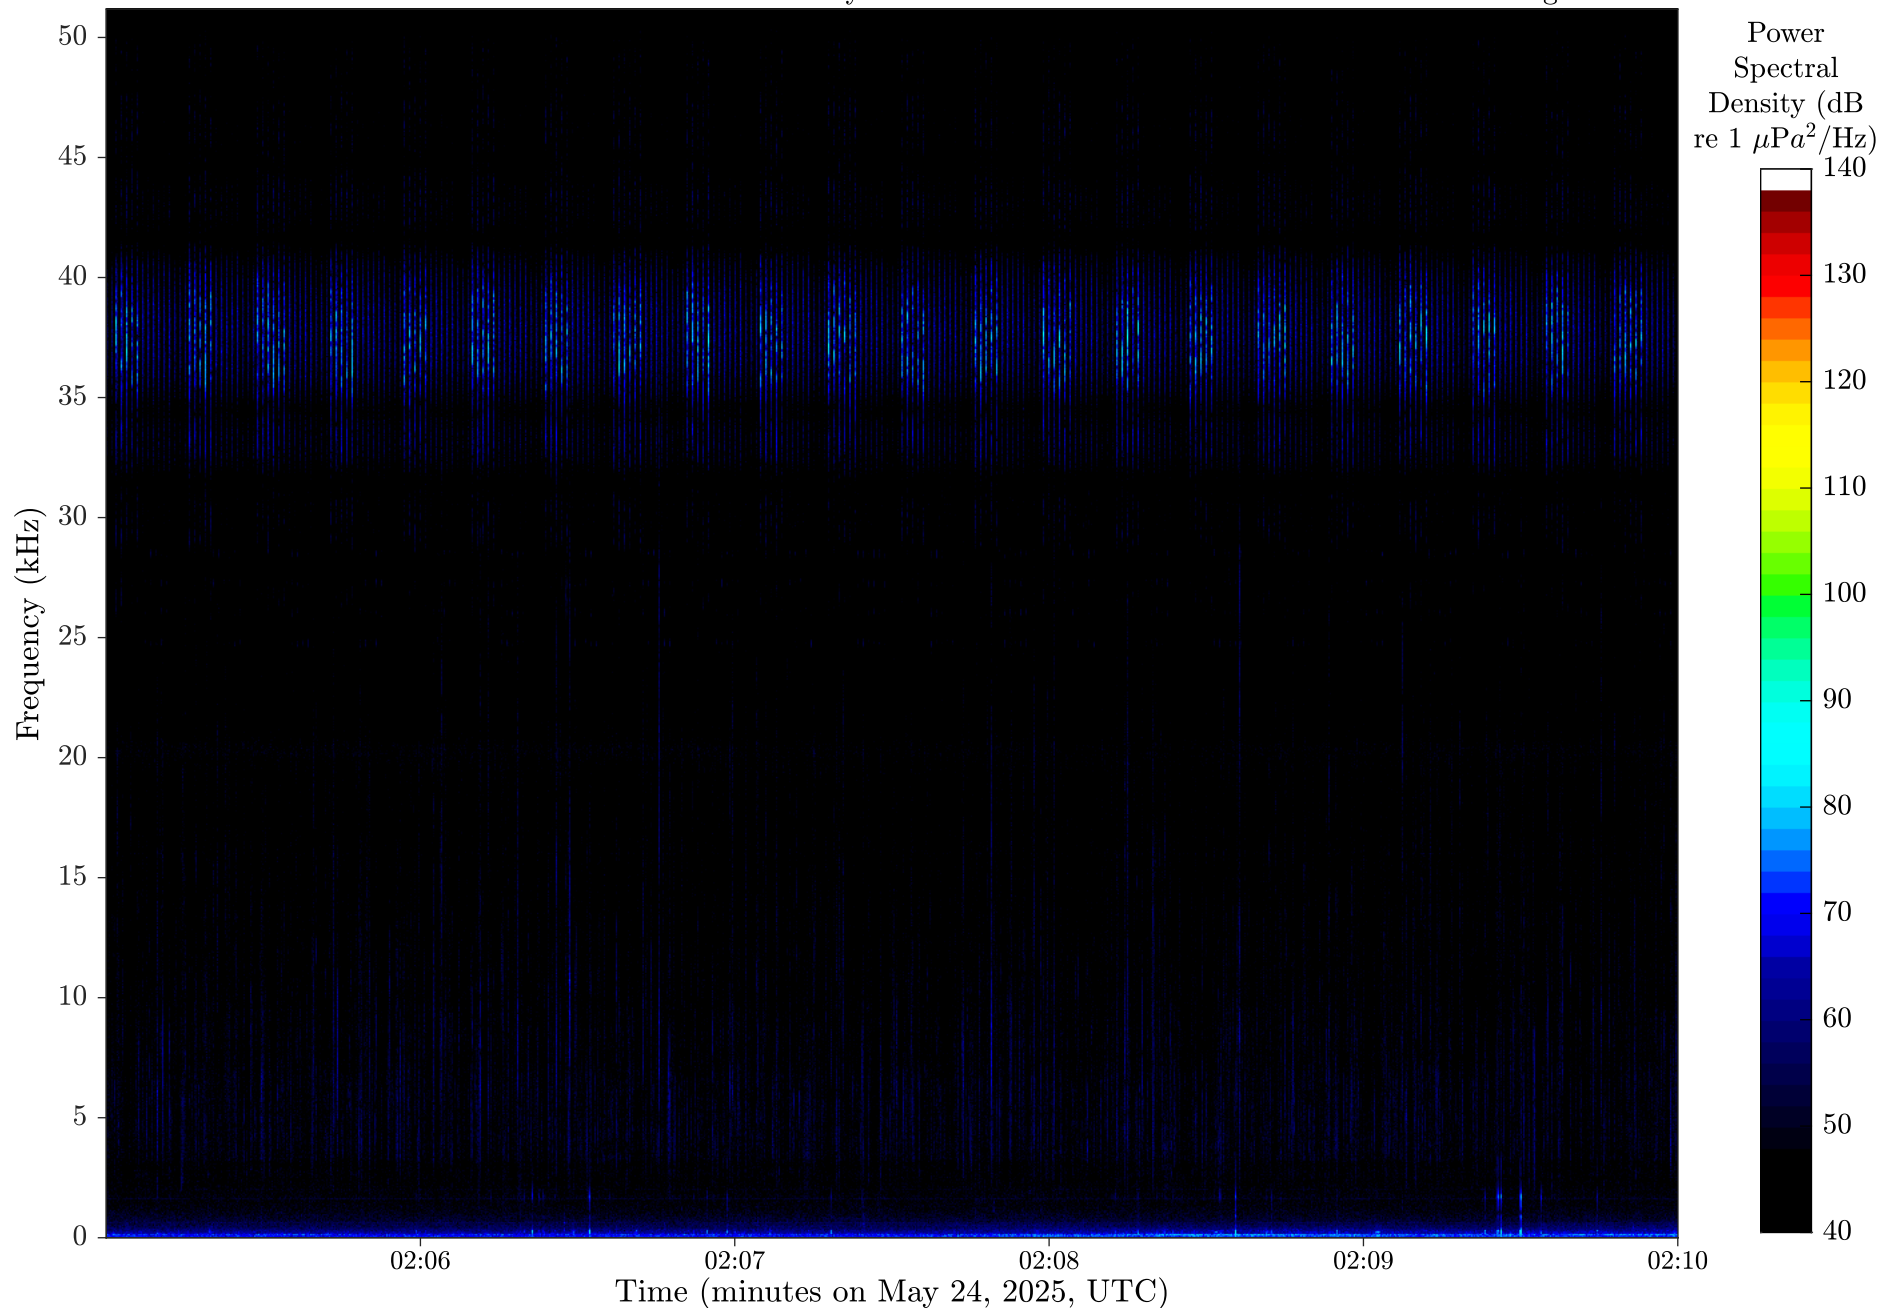


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:11:12 UTC

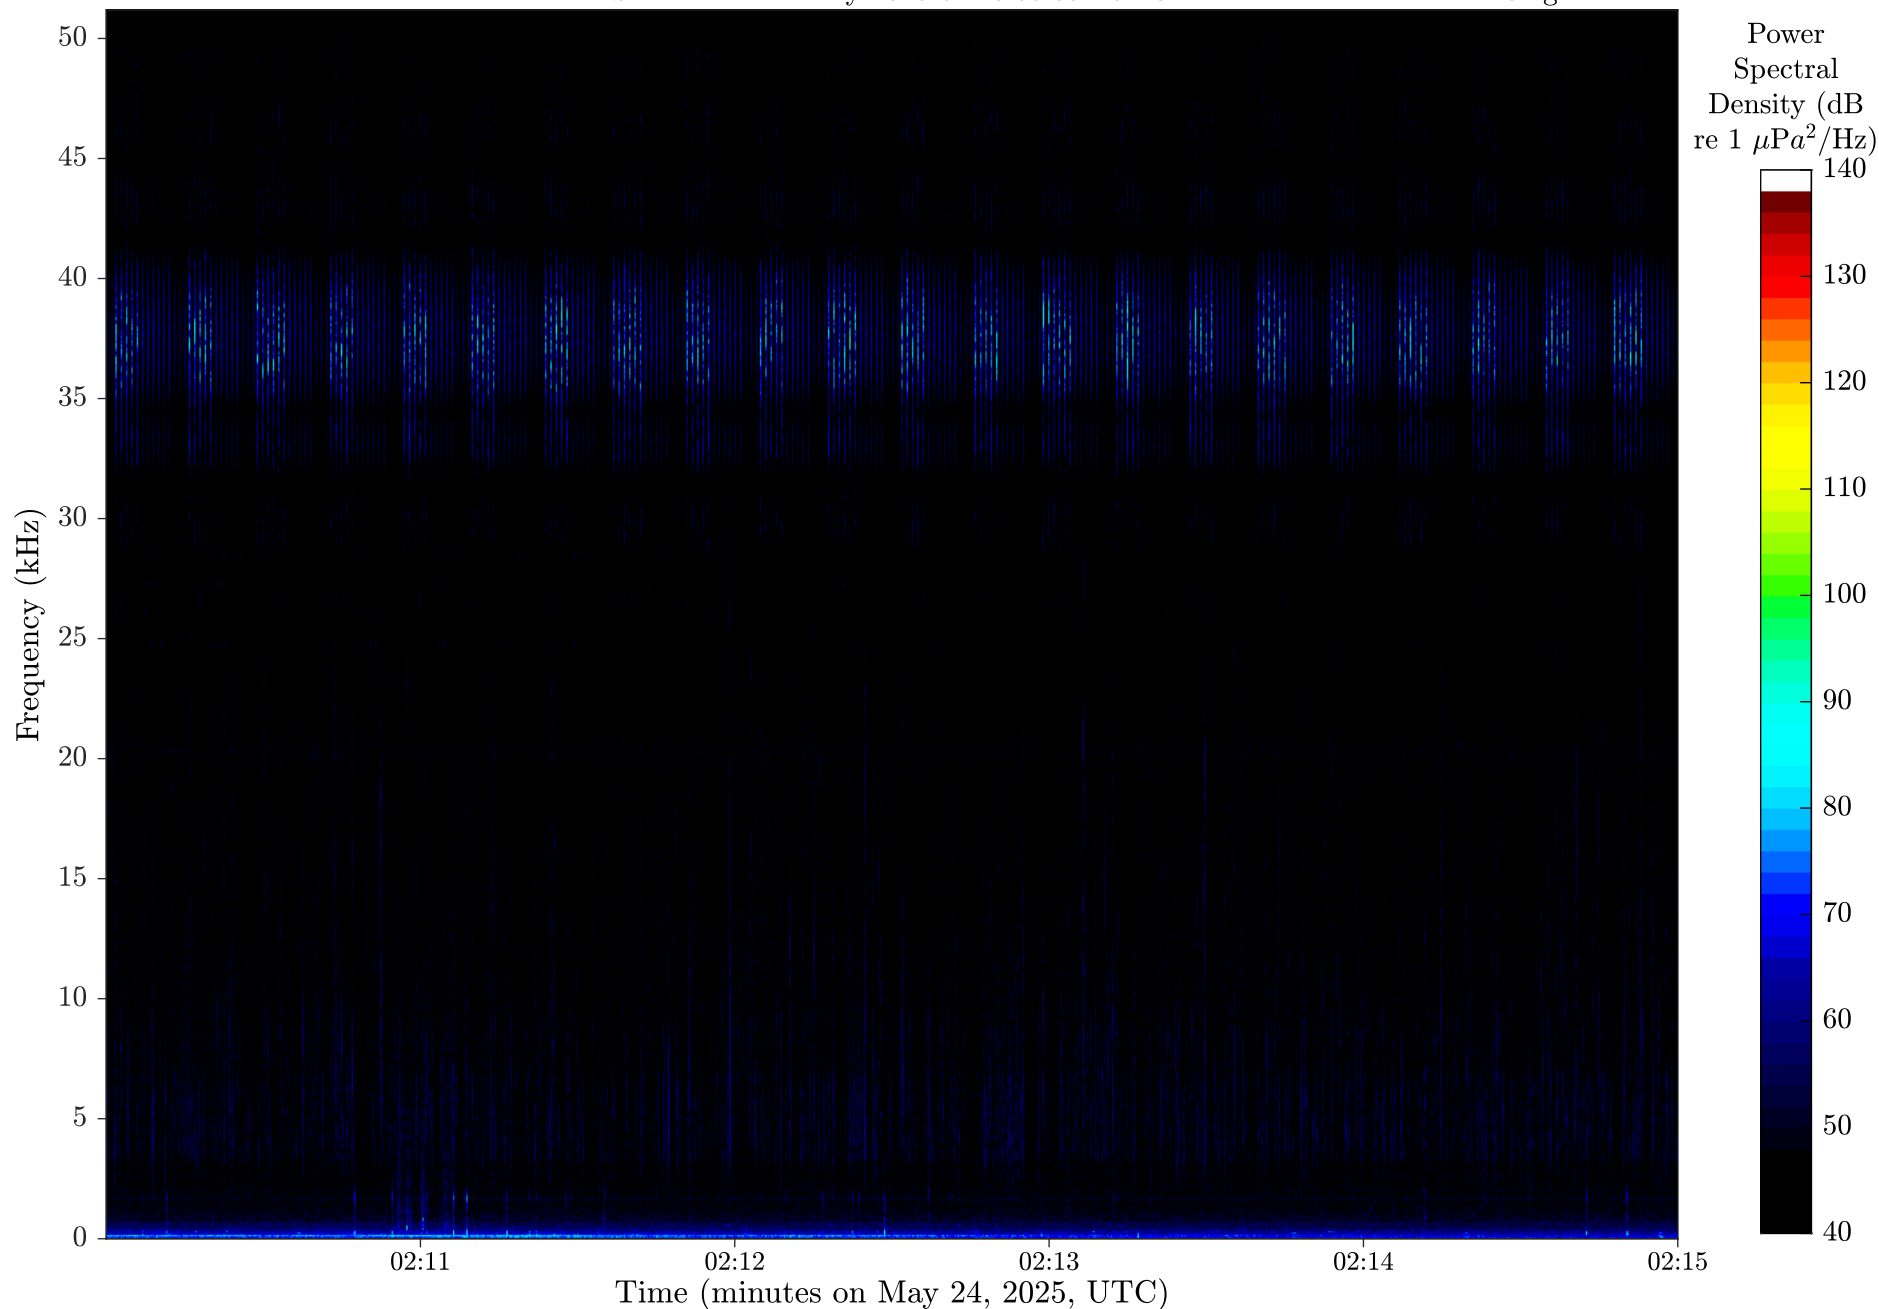


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:11:19 UTC

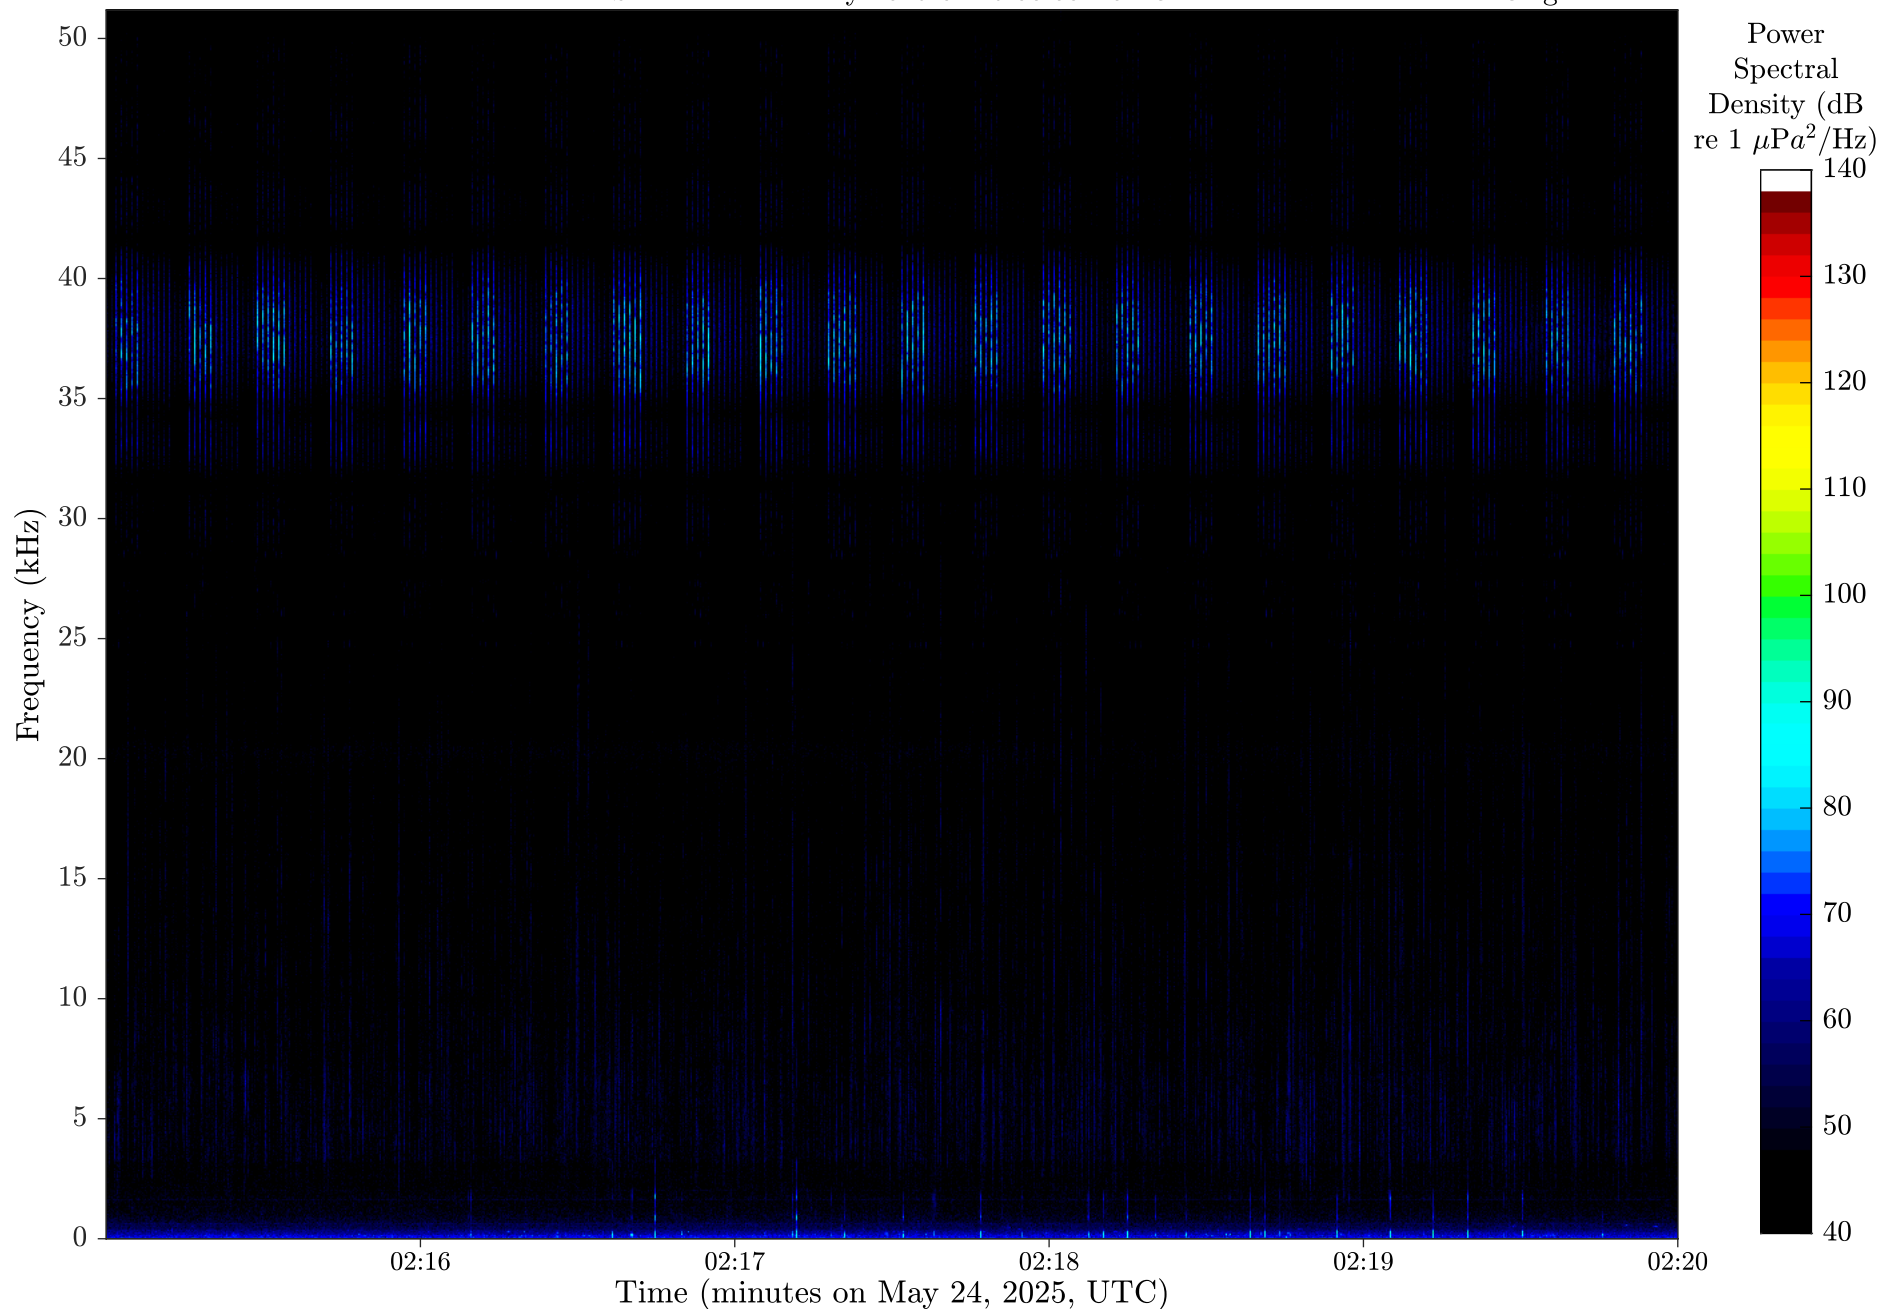


Comments: 35.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:11:27 UTC

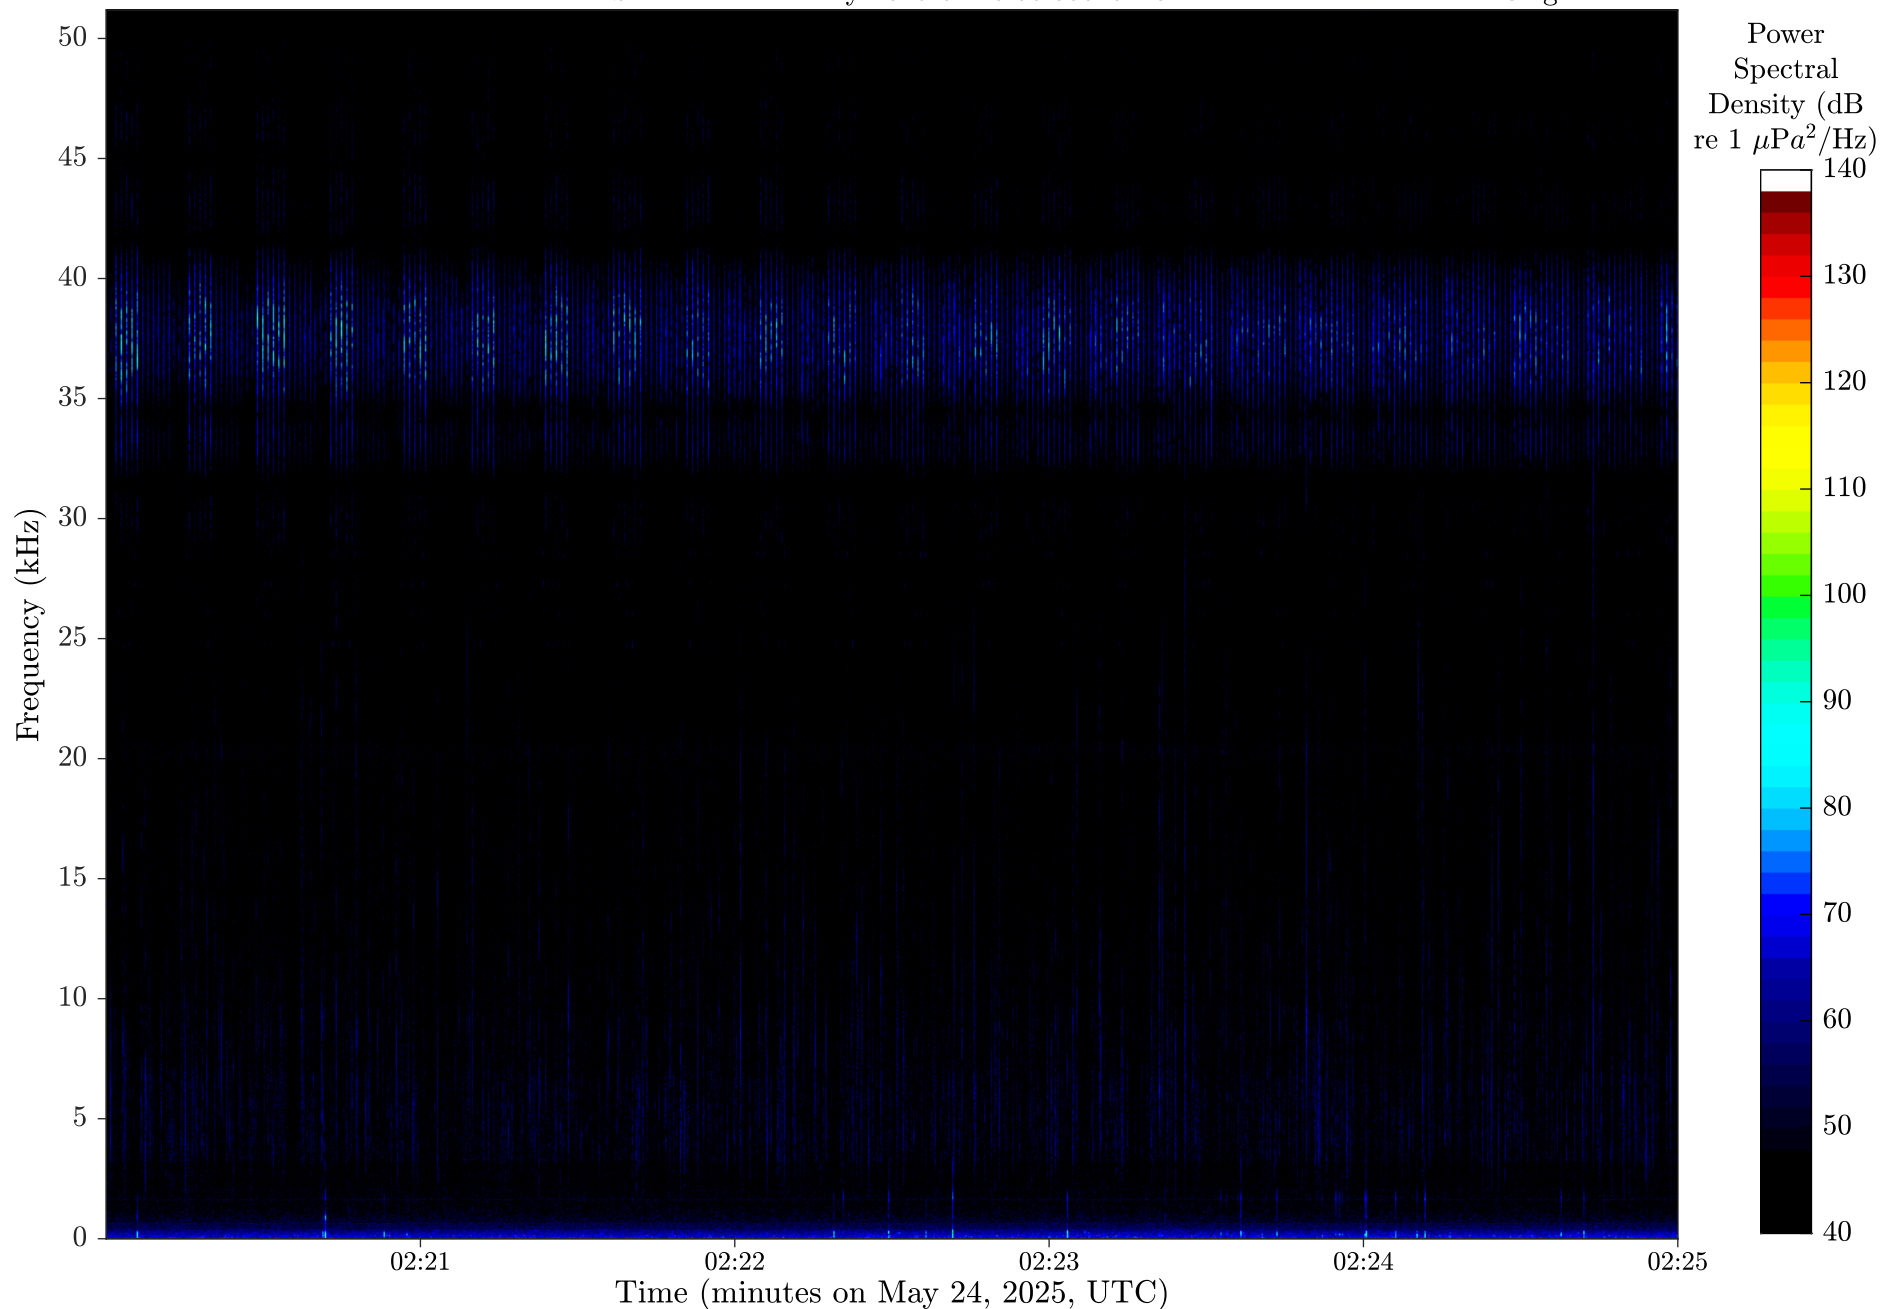


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:11:33 UTC

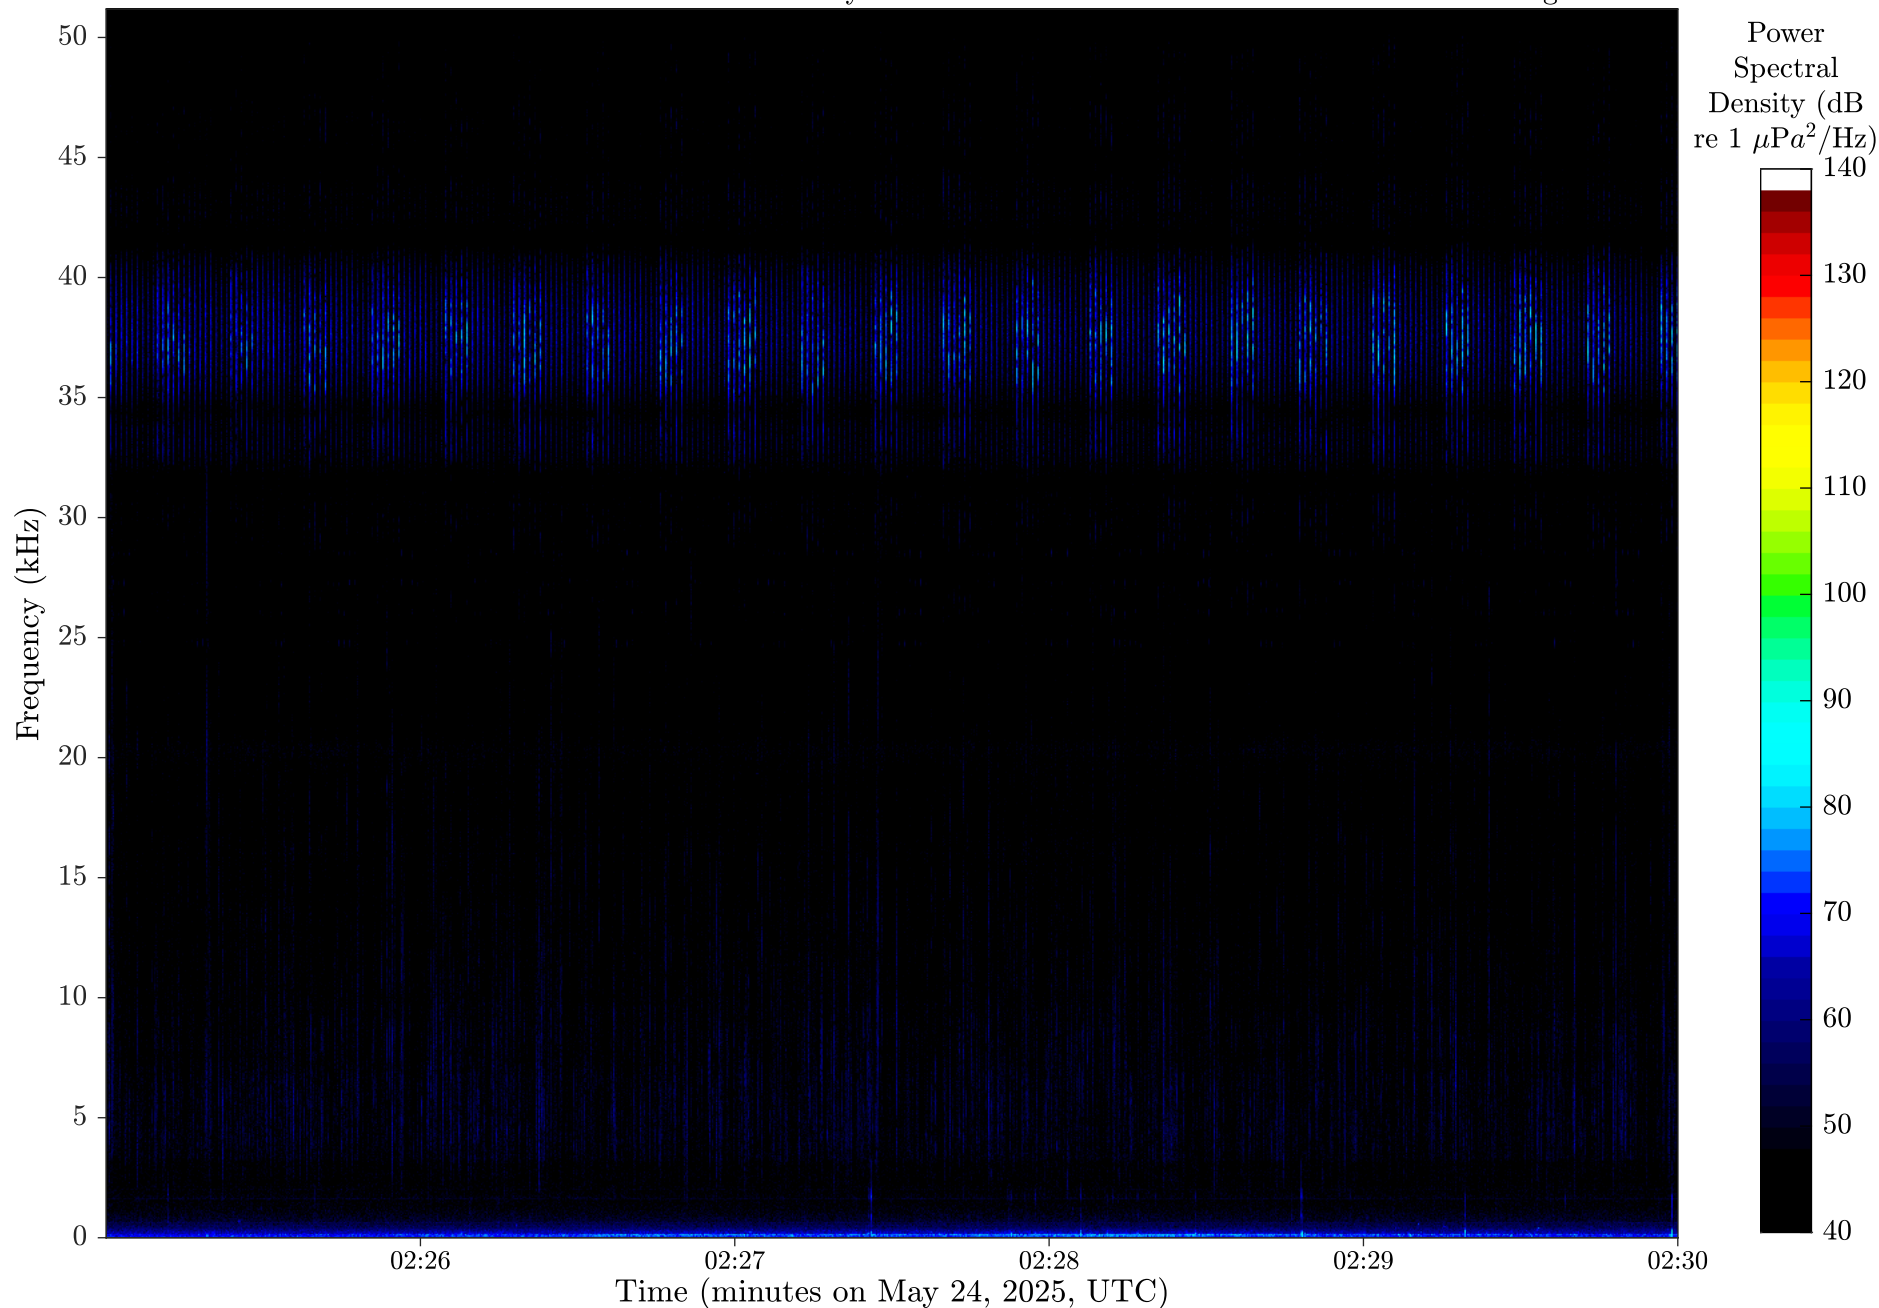

Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:11:41 UTC

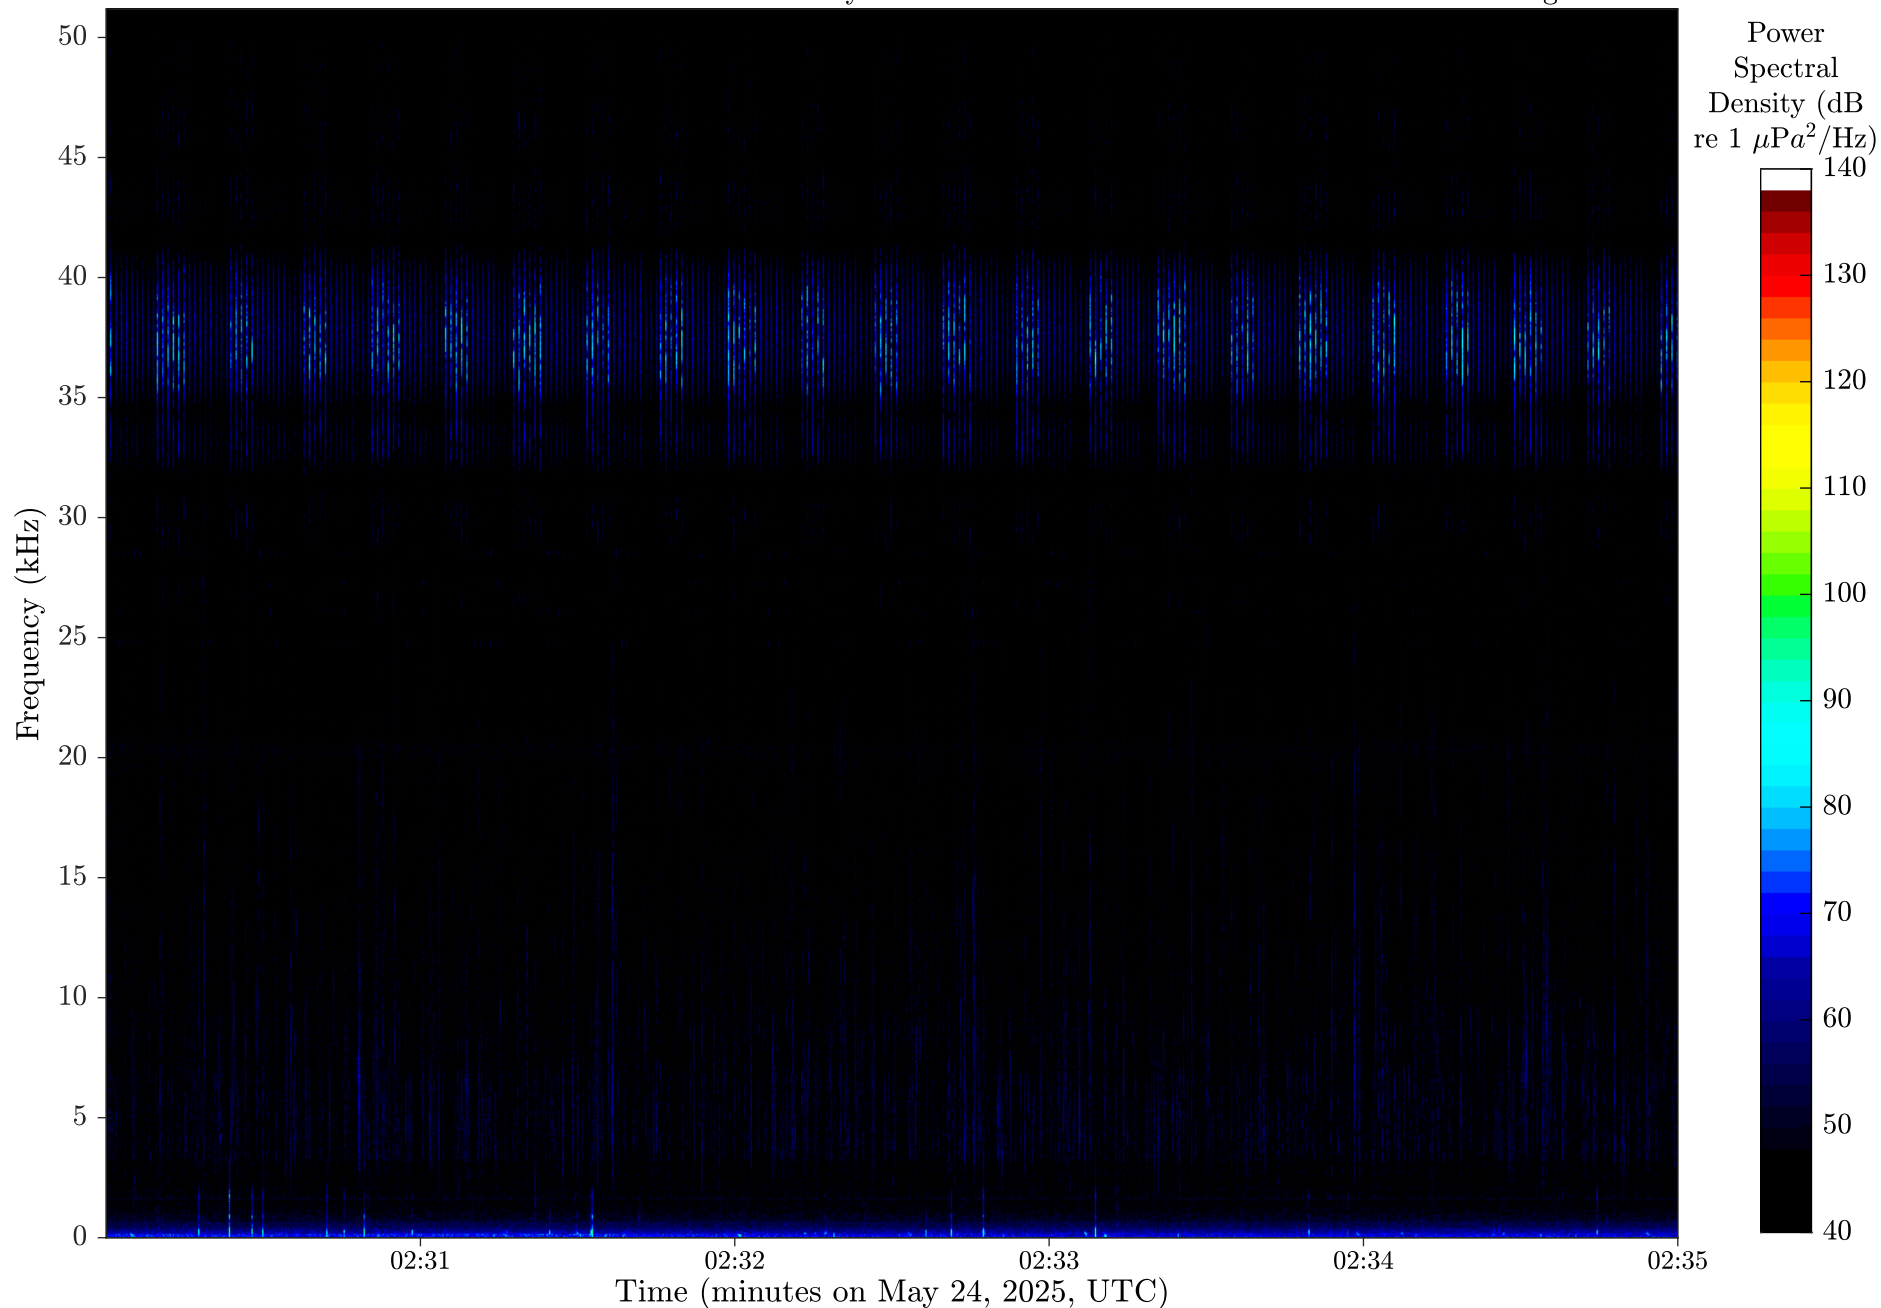

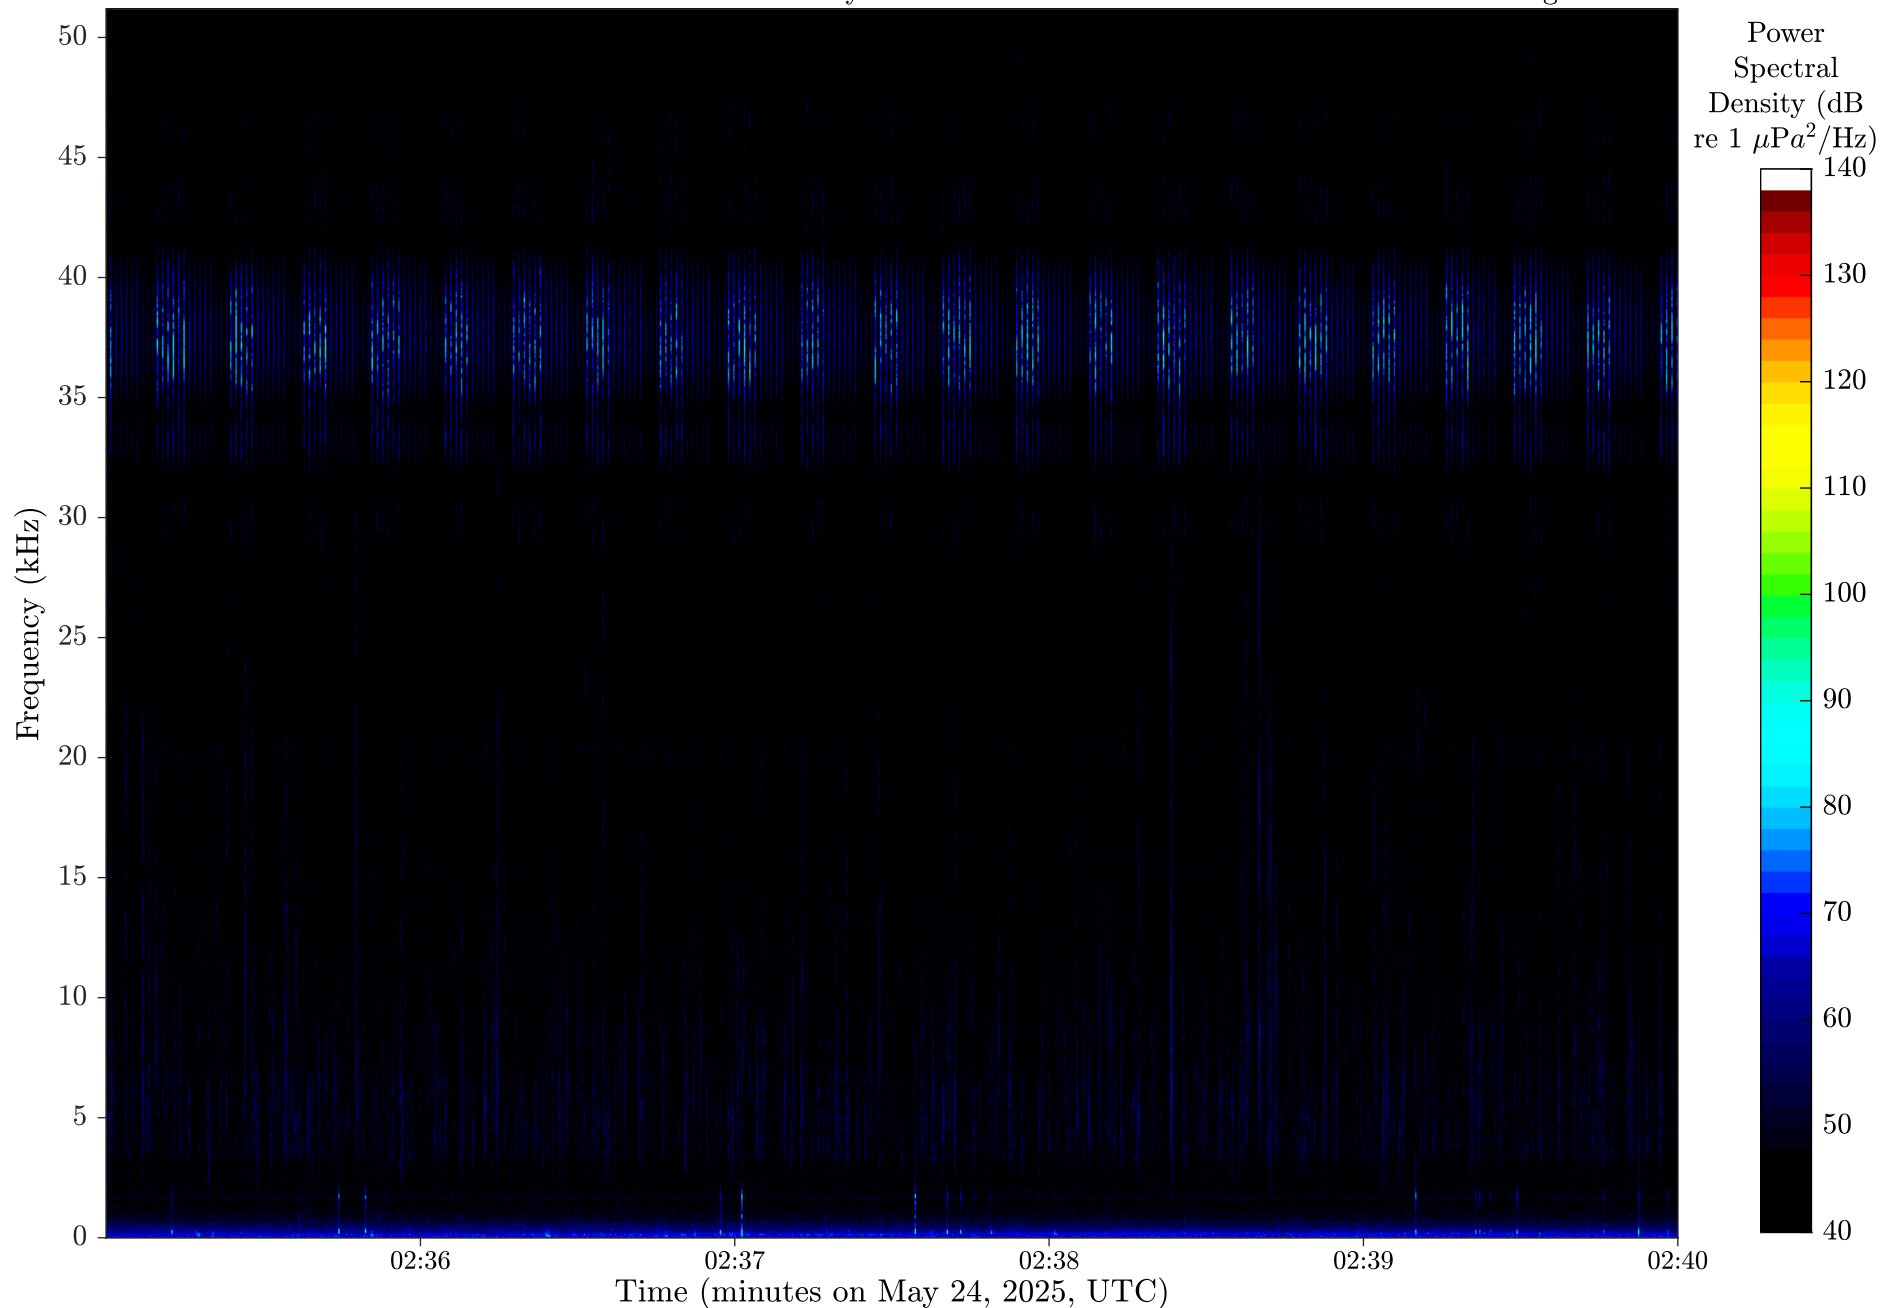


Comments: 36.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:11:56 UTC

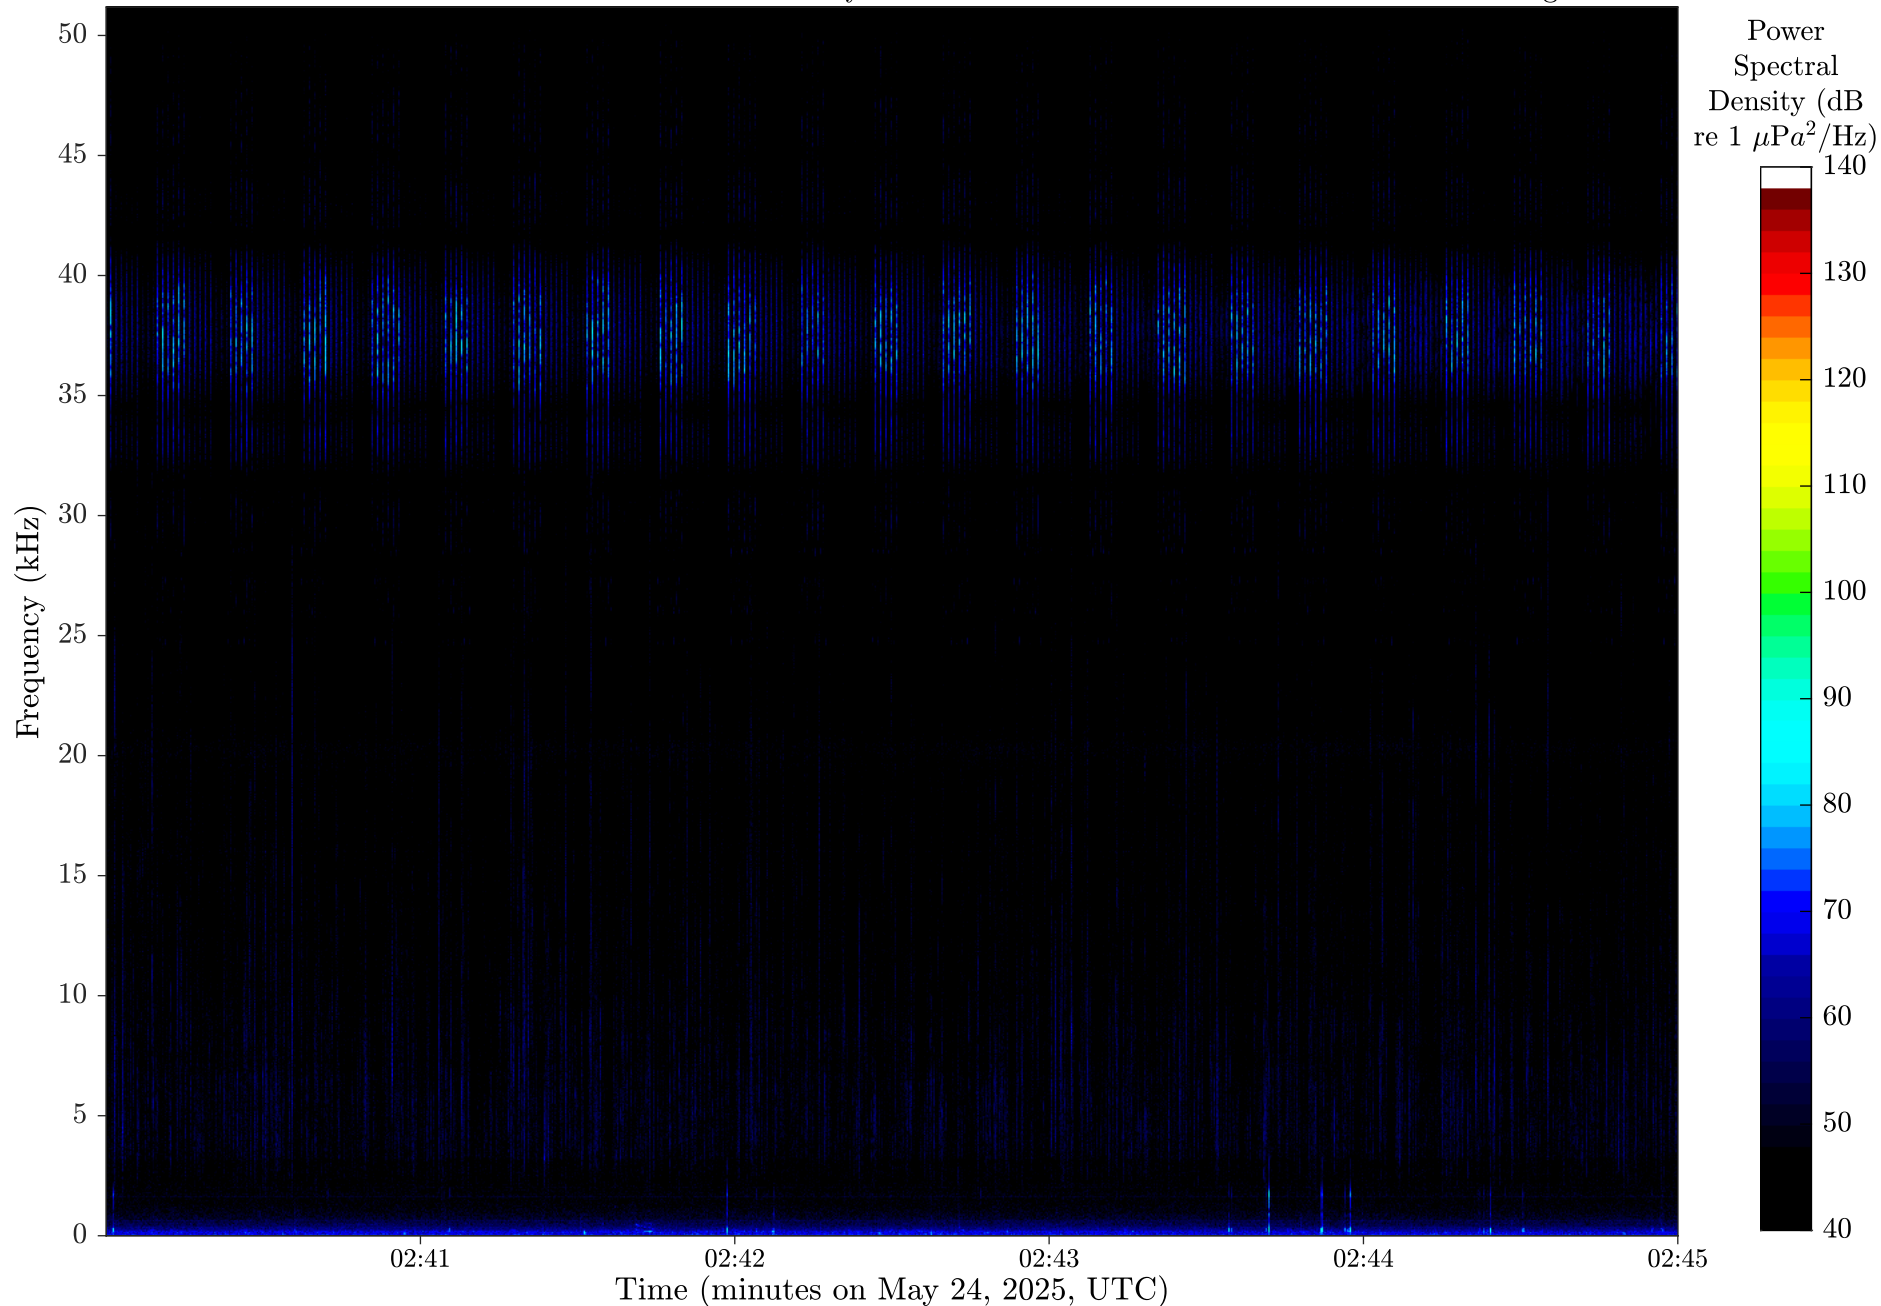


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:12:04 UTC

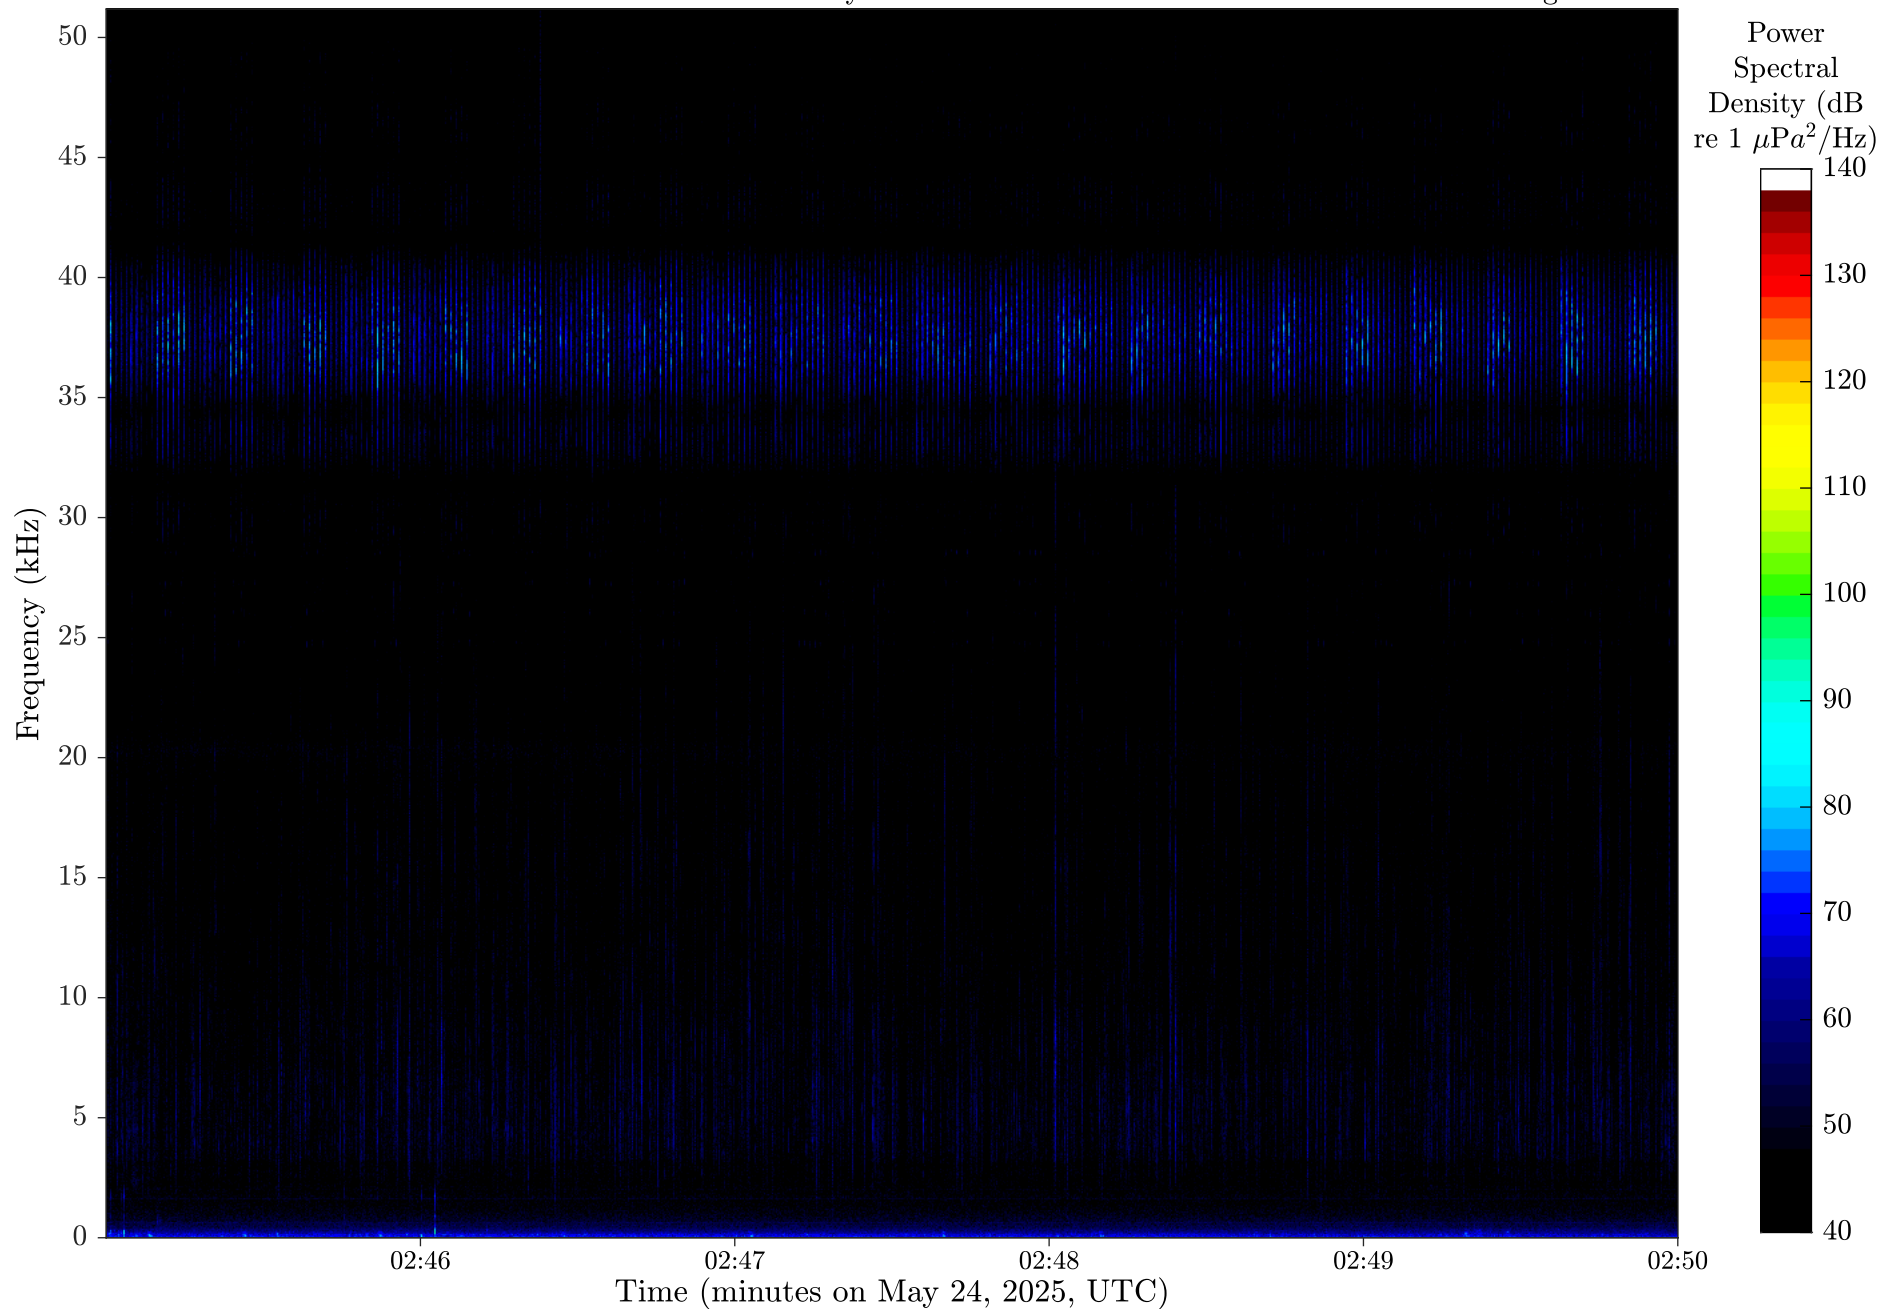


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:12:12 UTC

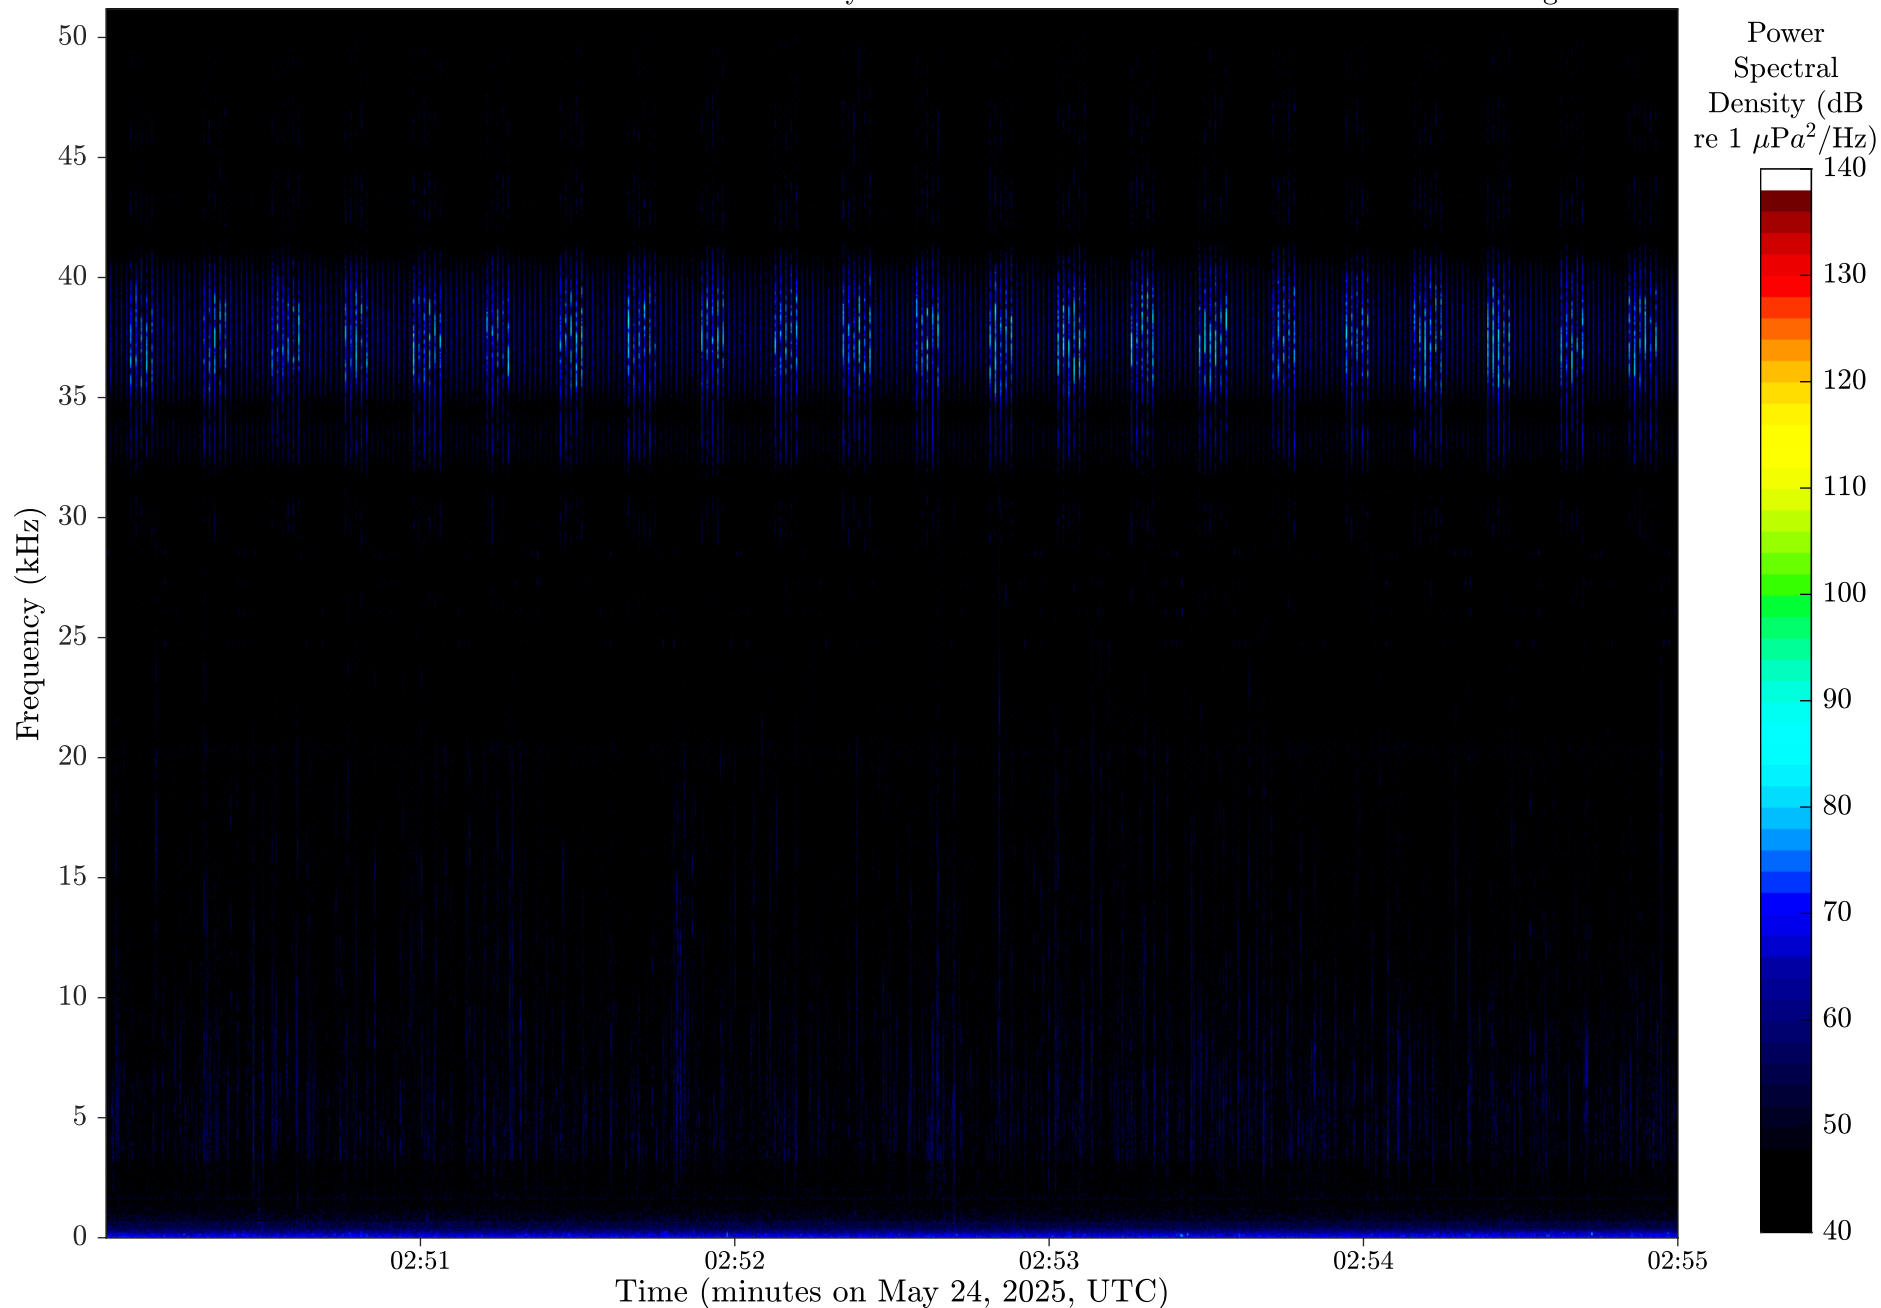


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:12:19 UTC

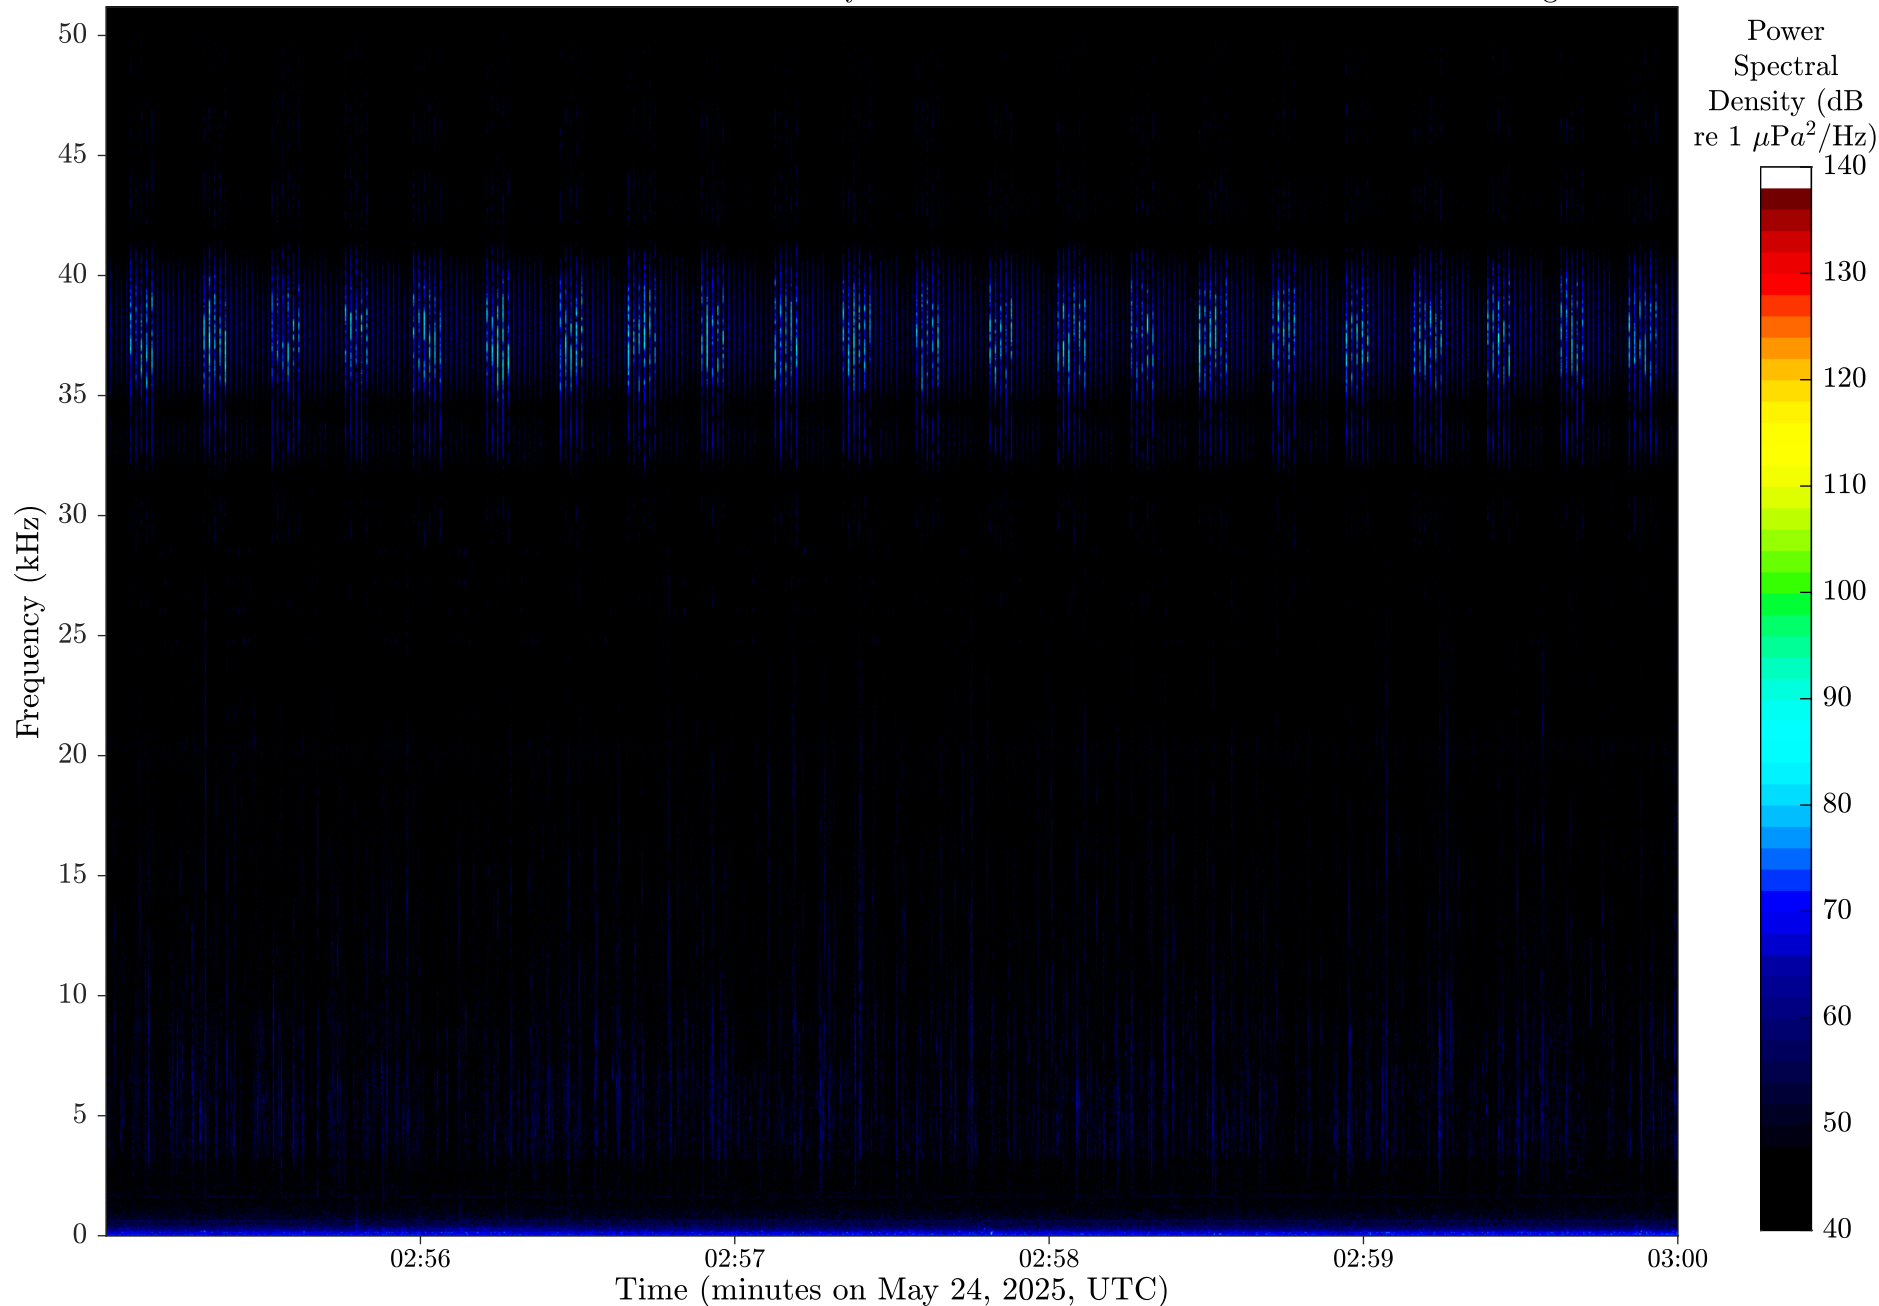


Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:12:27 UTC

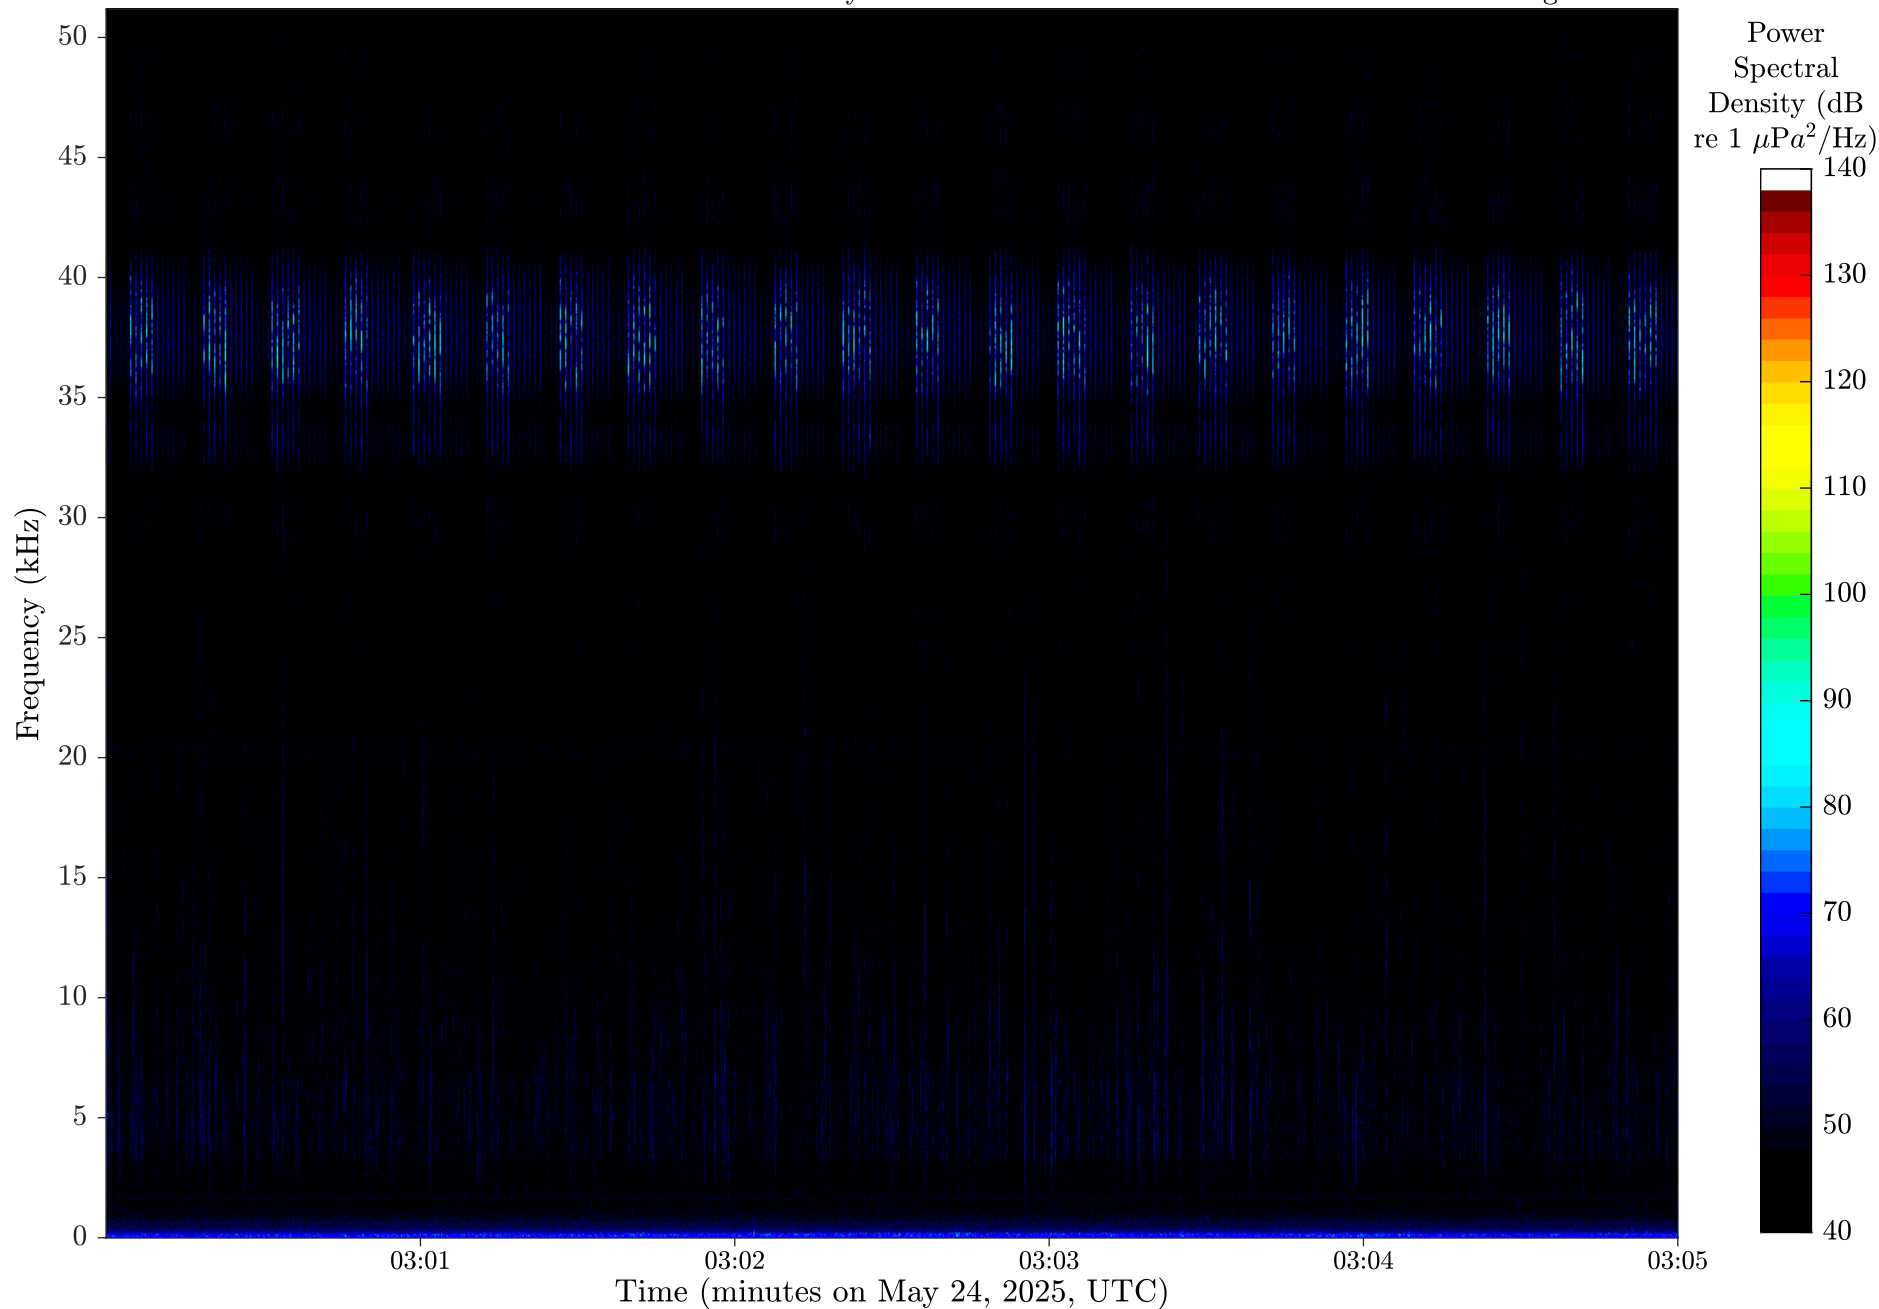


Comments: 35.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:12:35 UTC

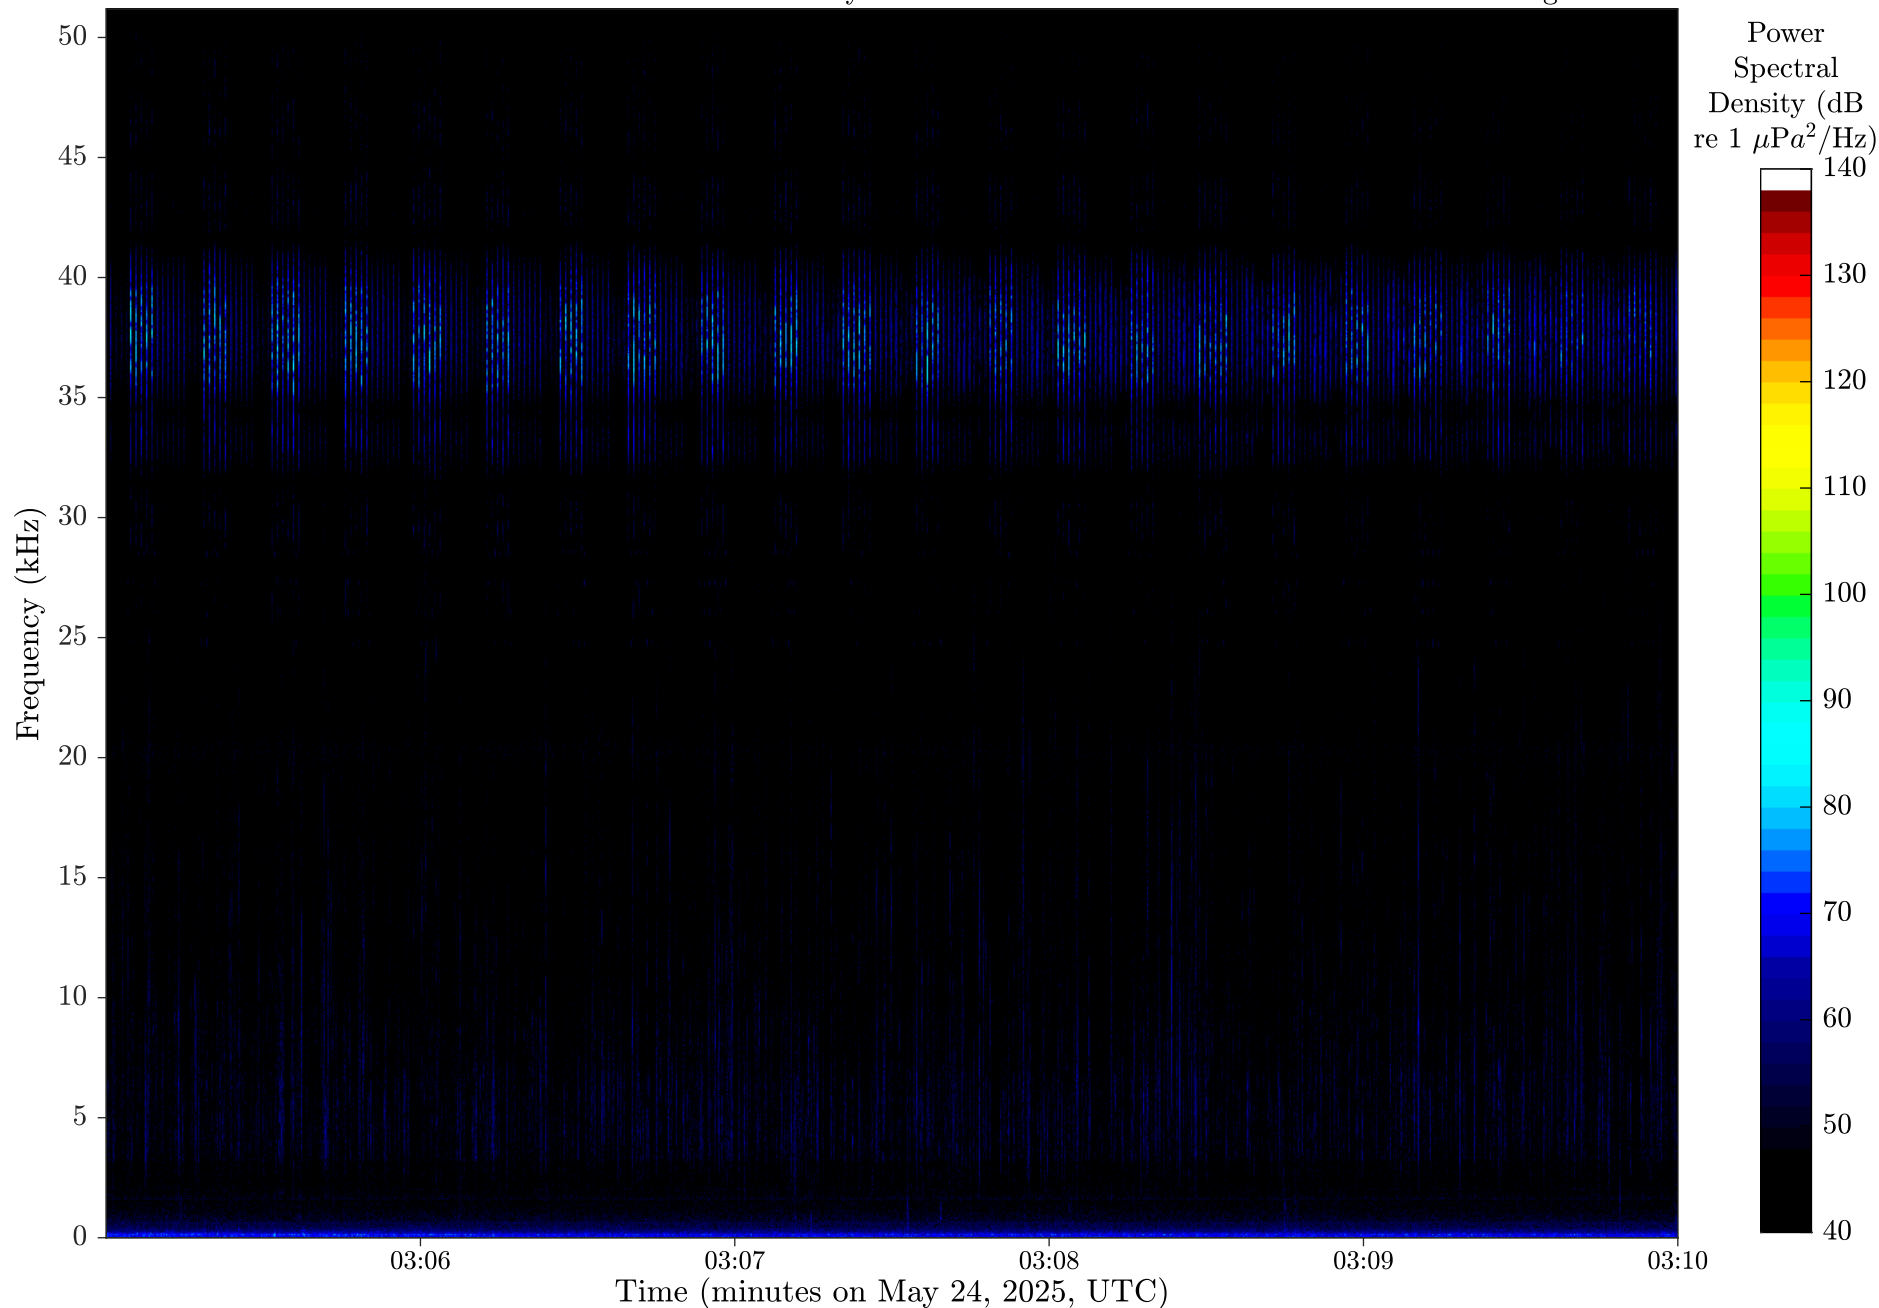


Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:12:43 UTC

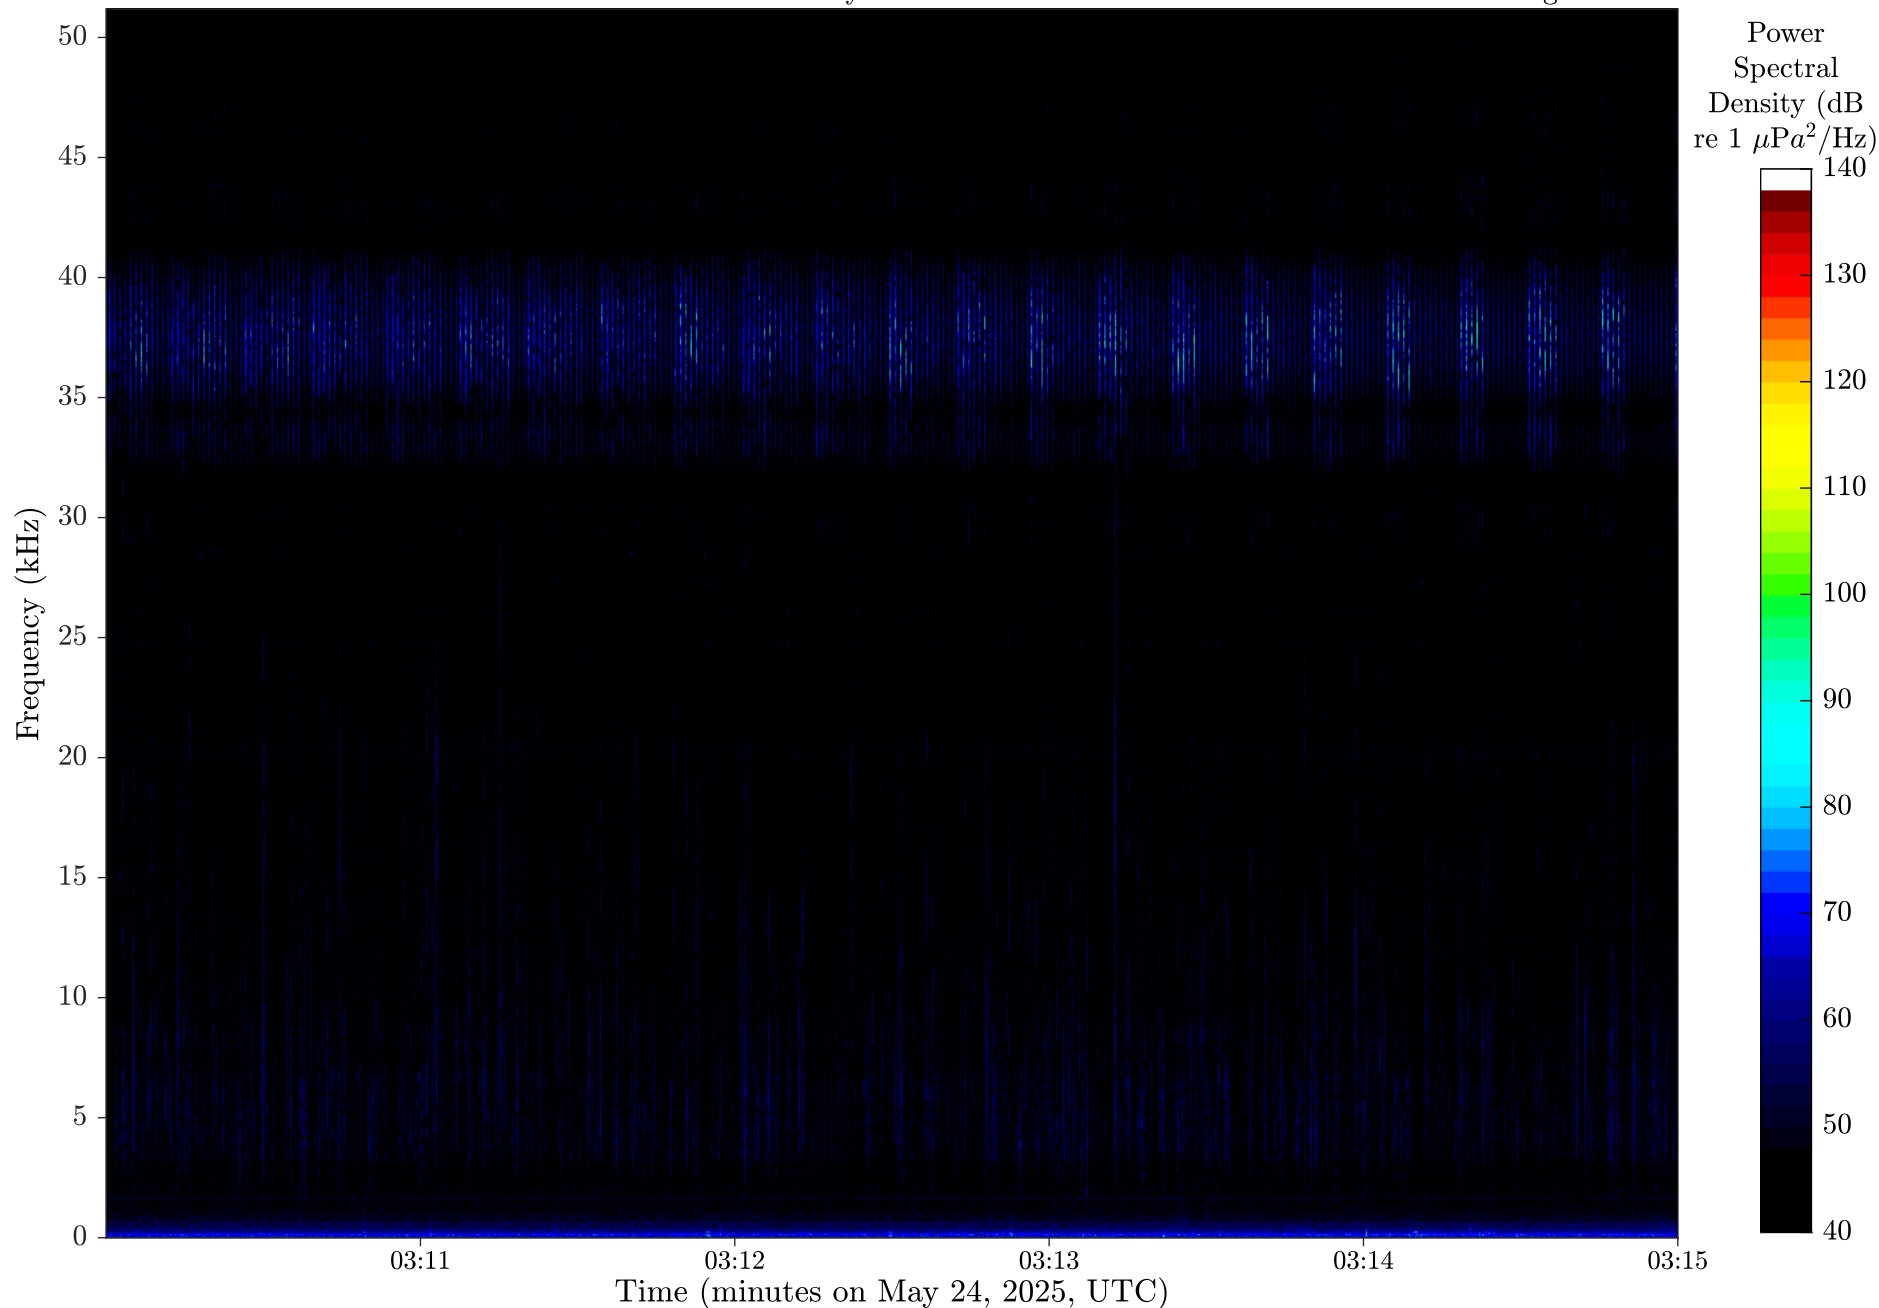


Comments: 33.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:12:51 UTC

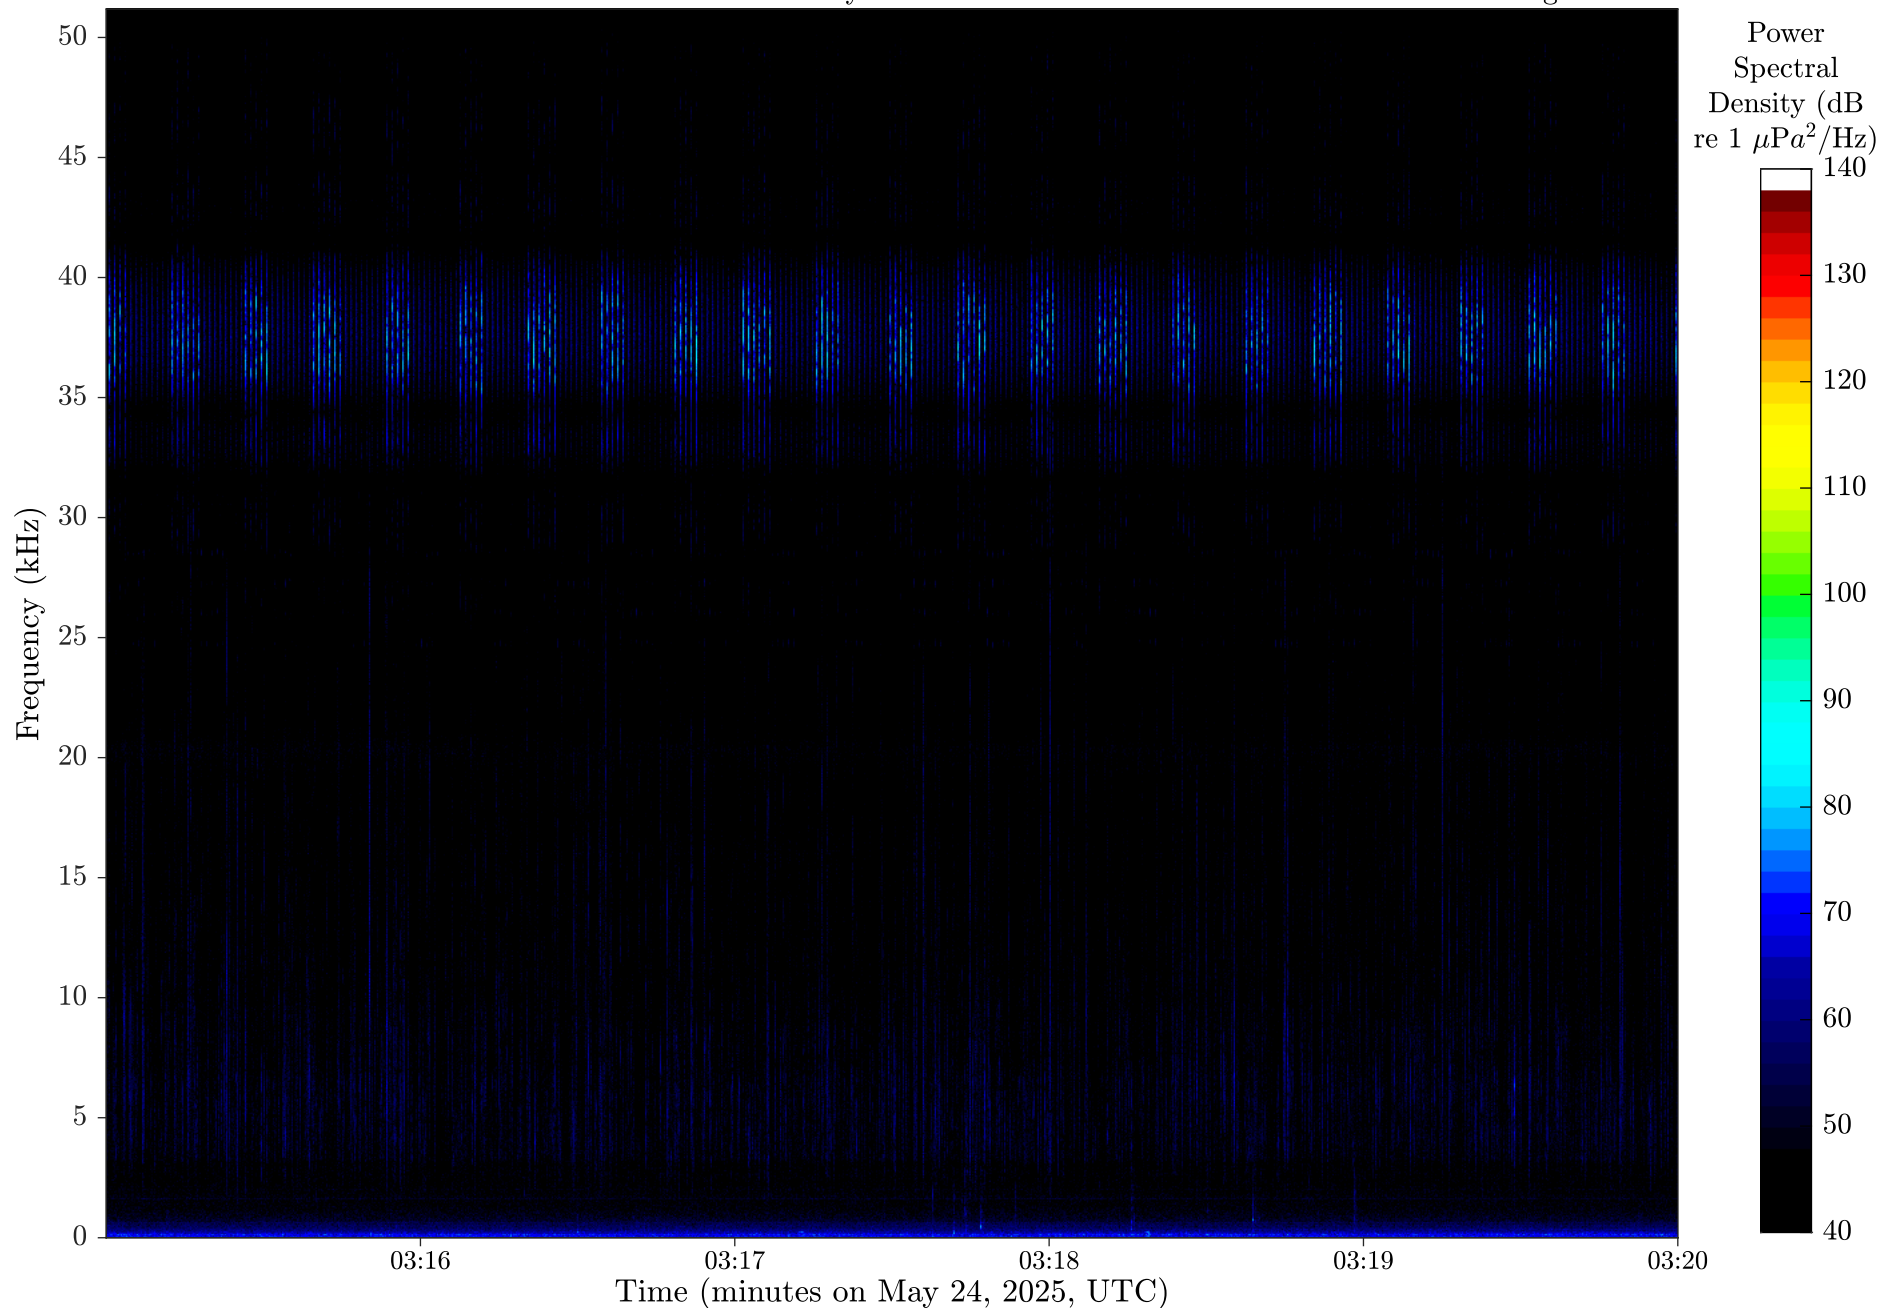


Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:12:59 UTC

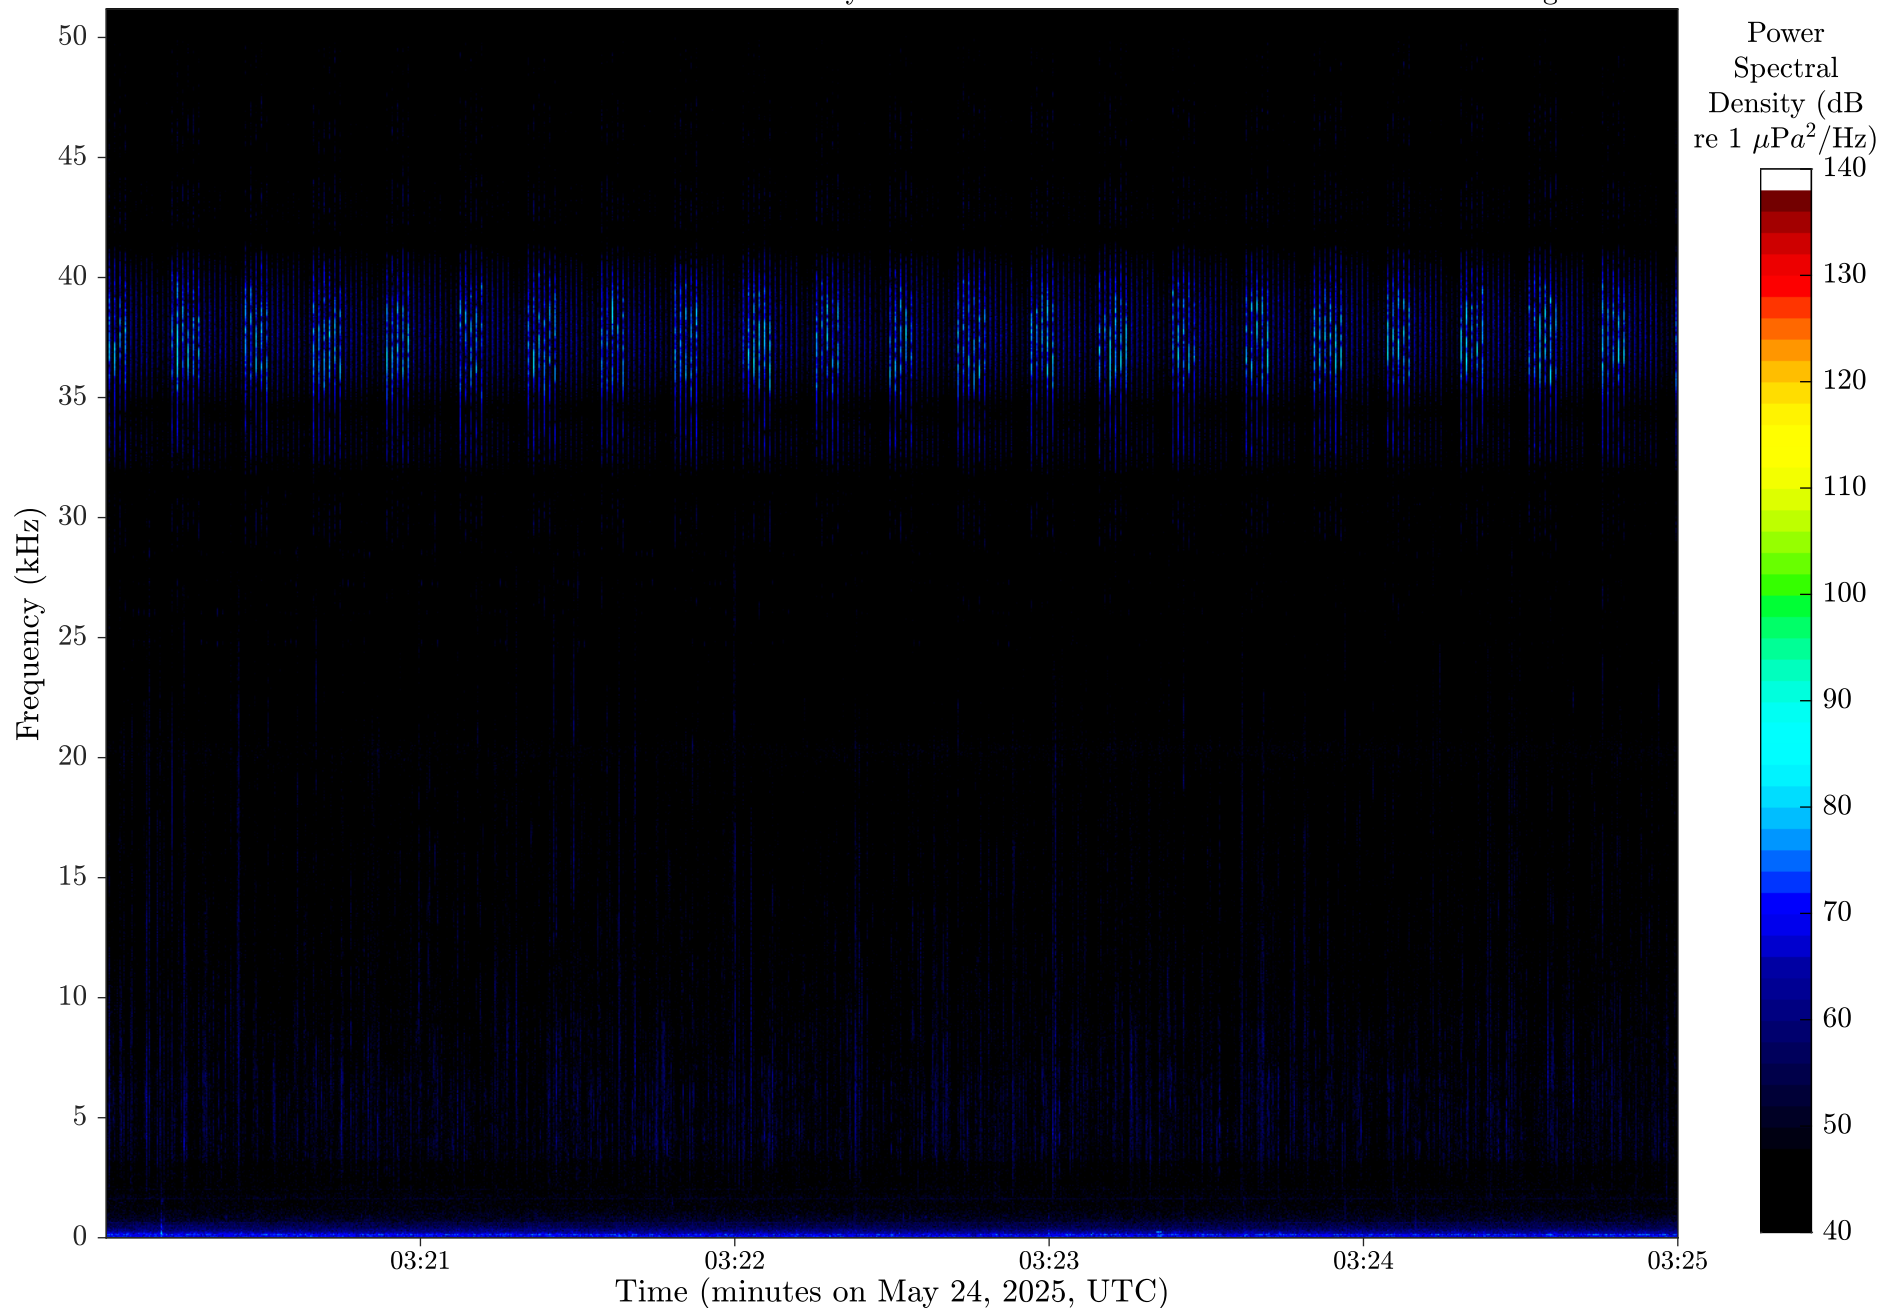


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:13:07 UTC

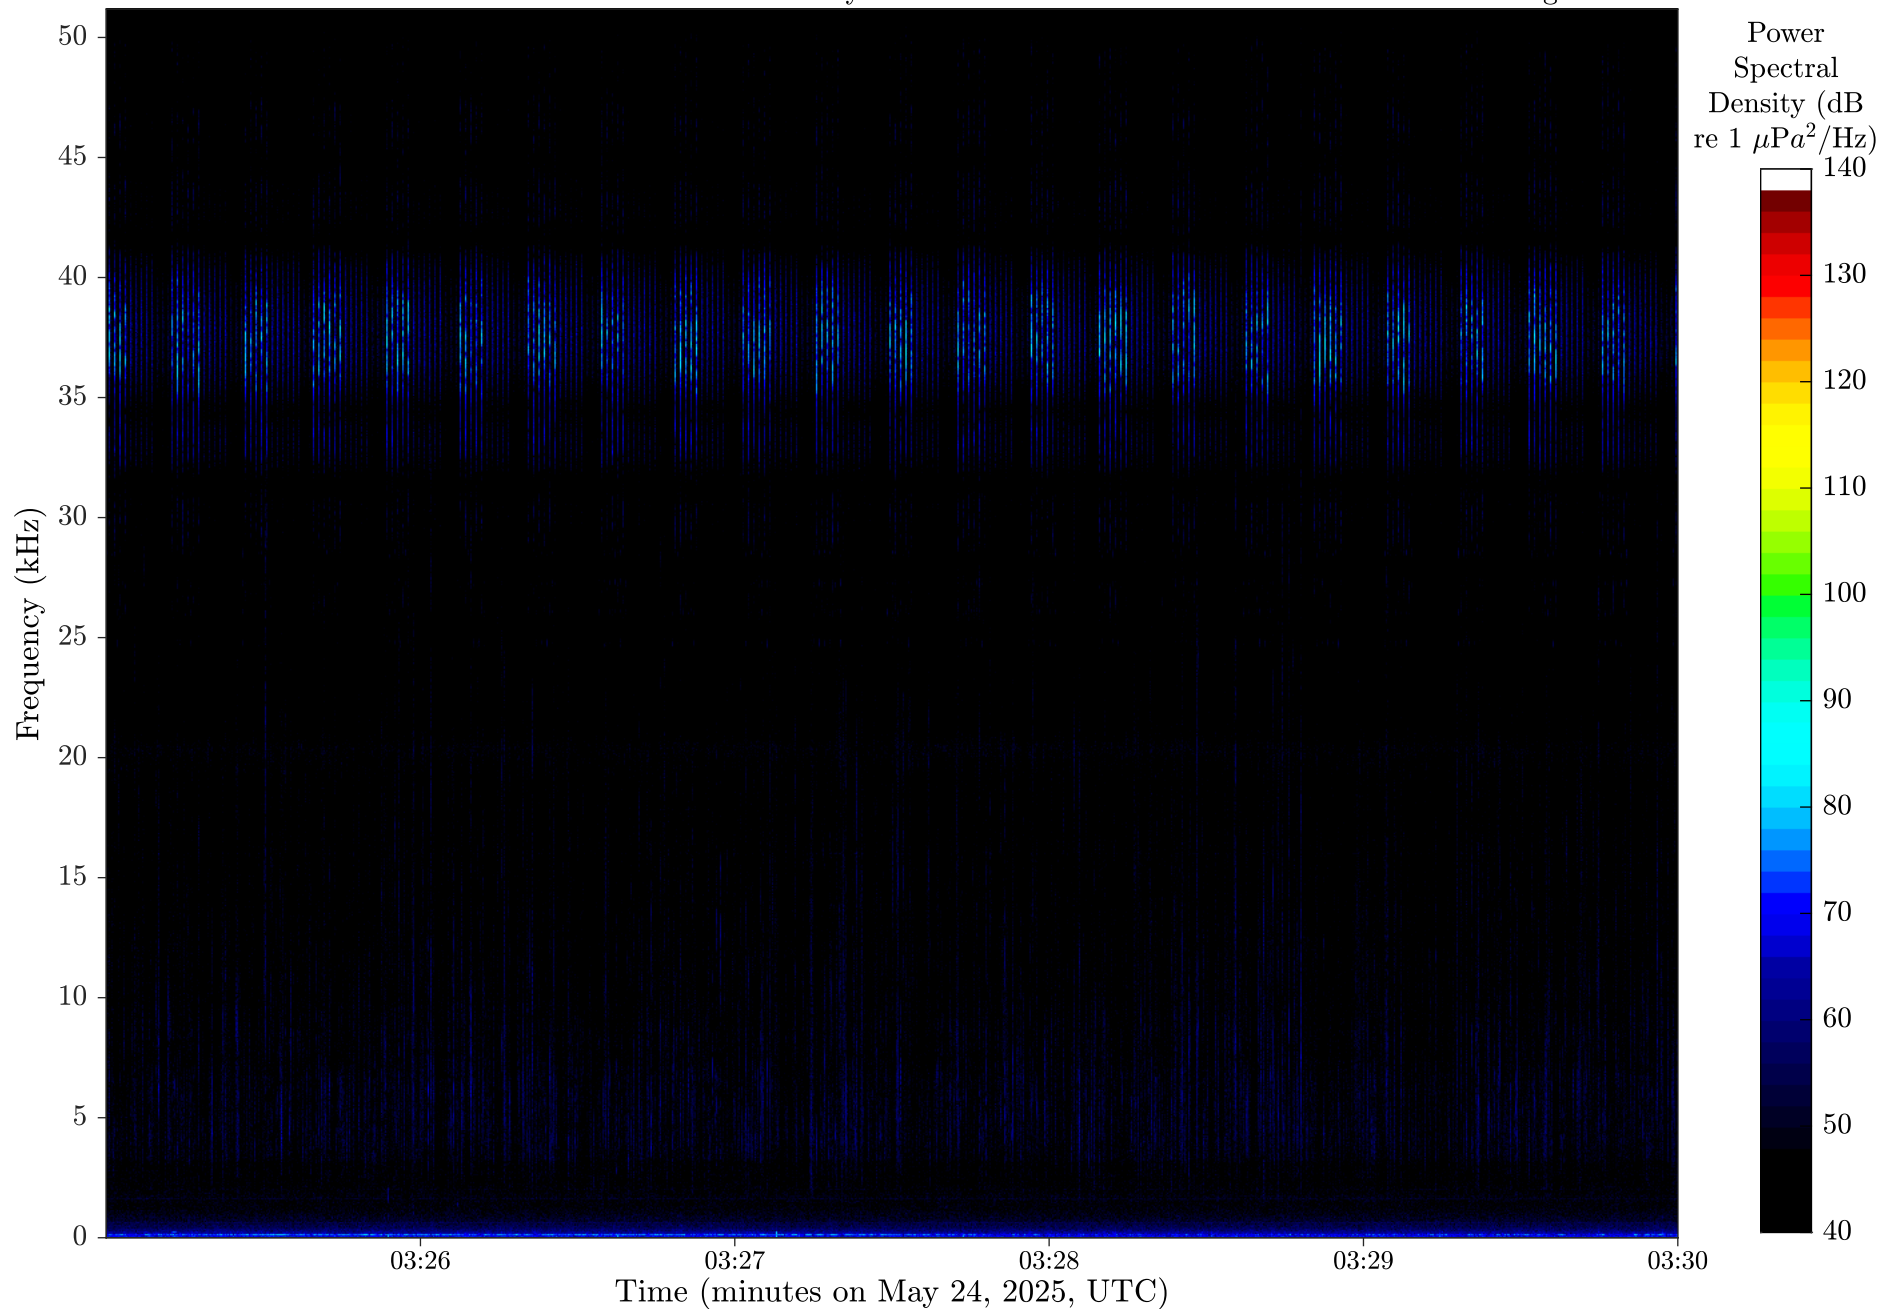


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:13:15 UTC

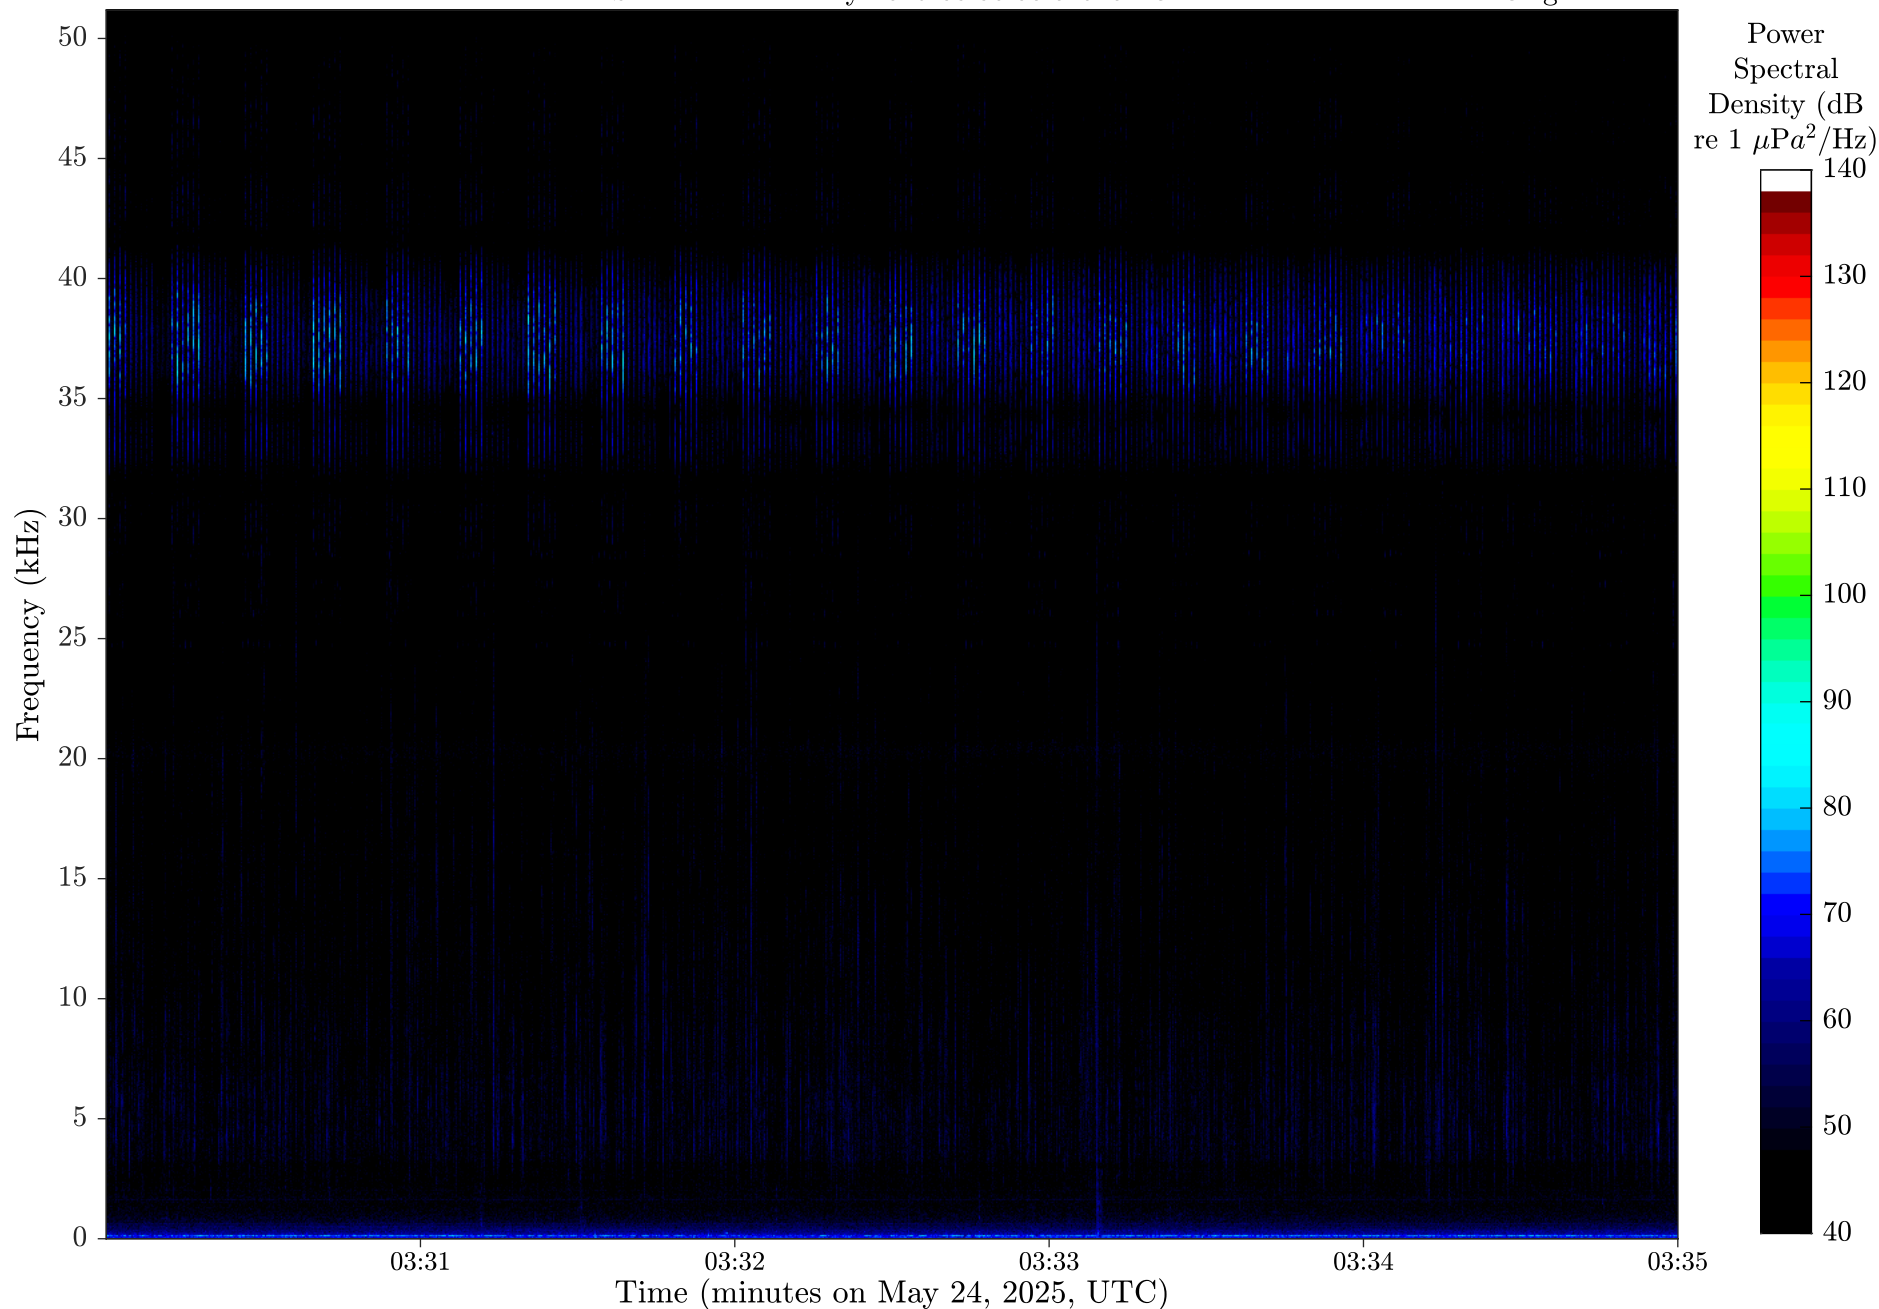


Comments: 34.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:13:23 UTC

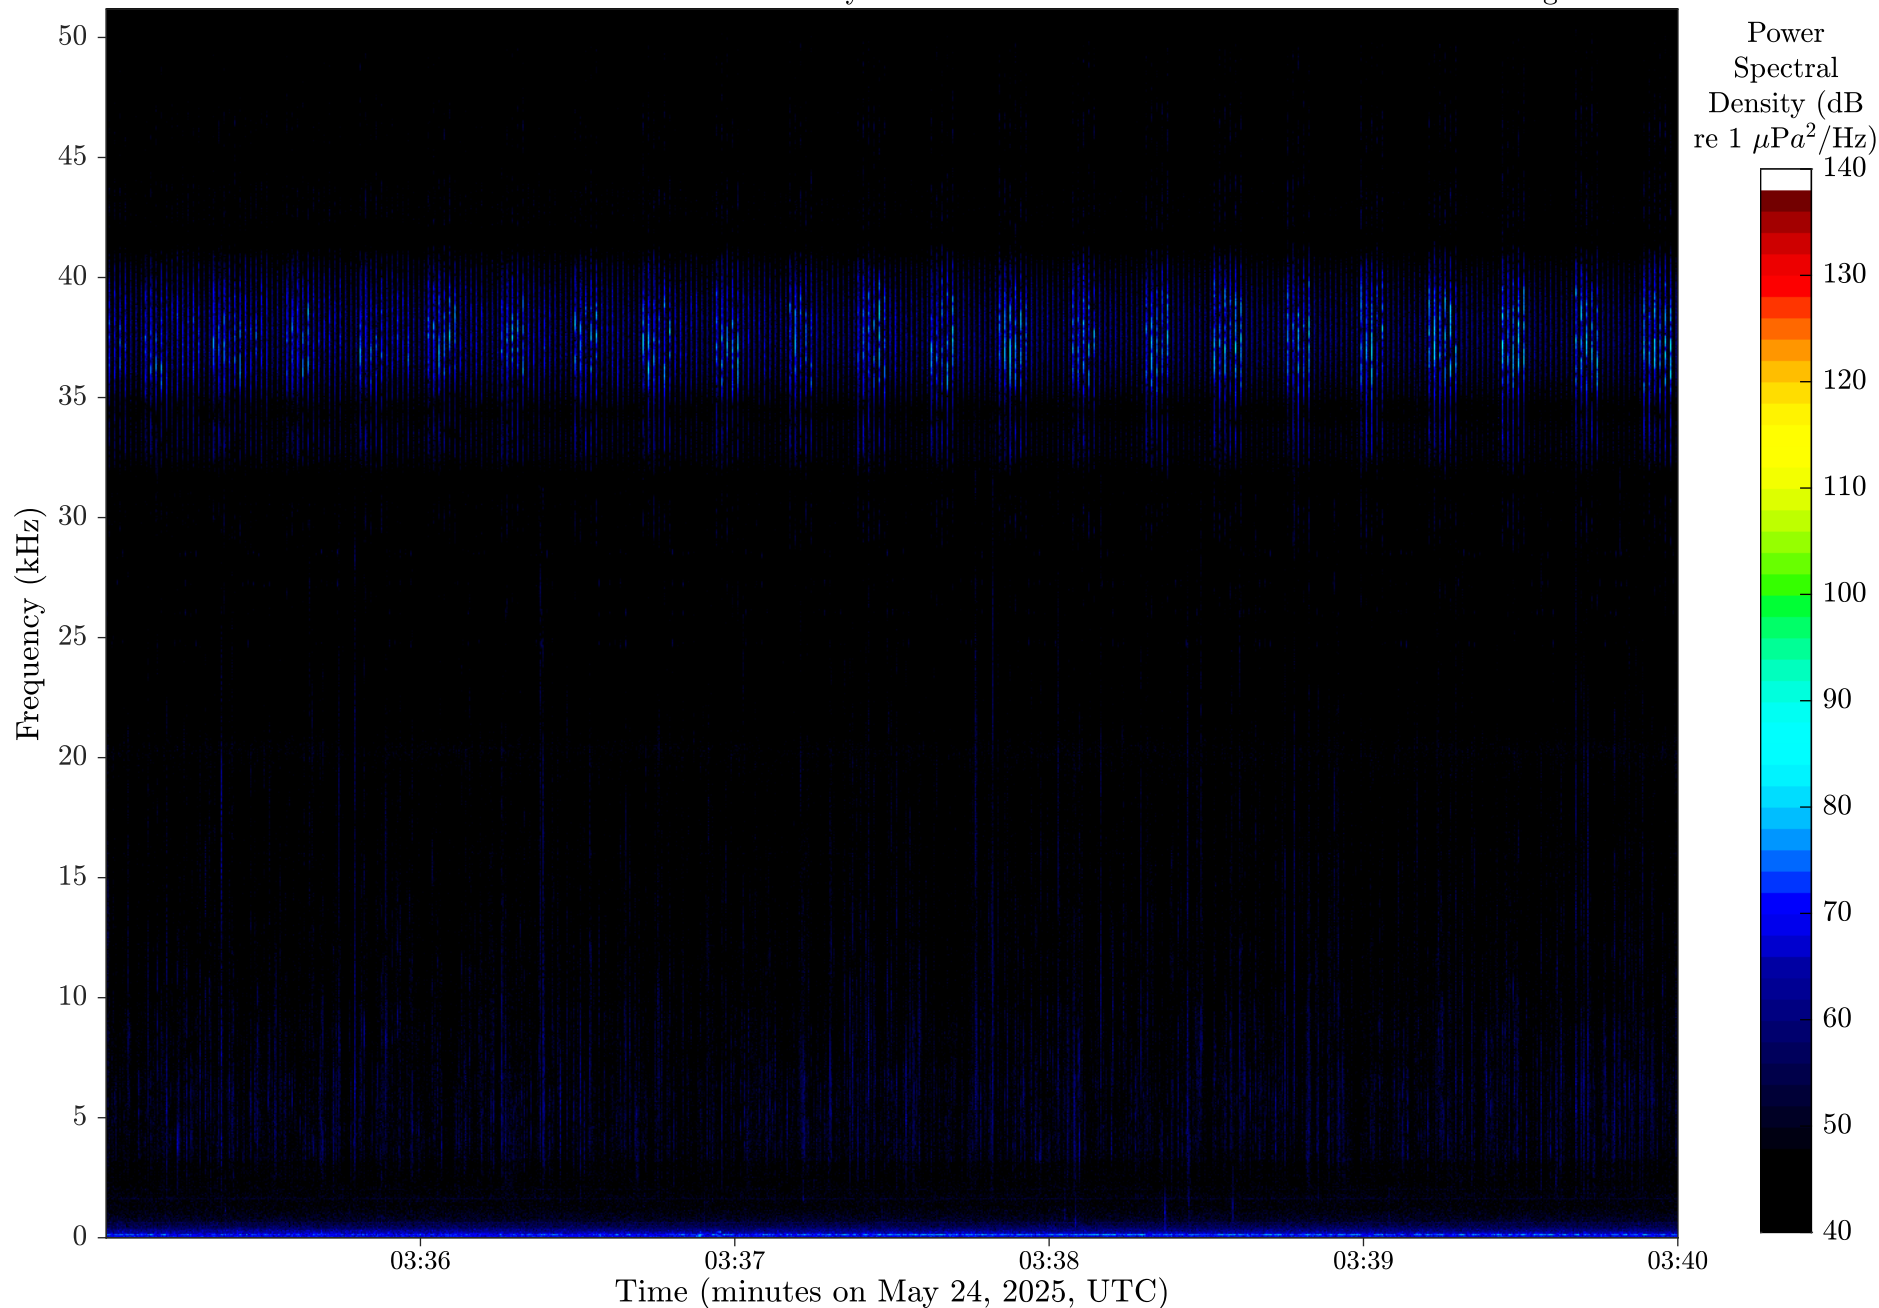

Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:13:31 UTC

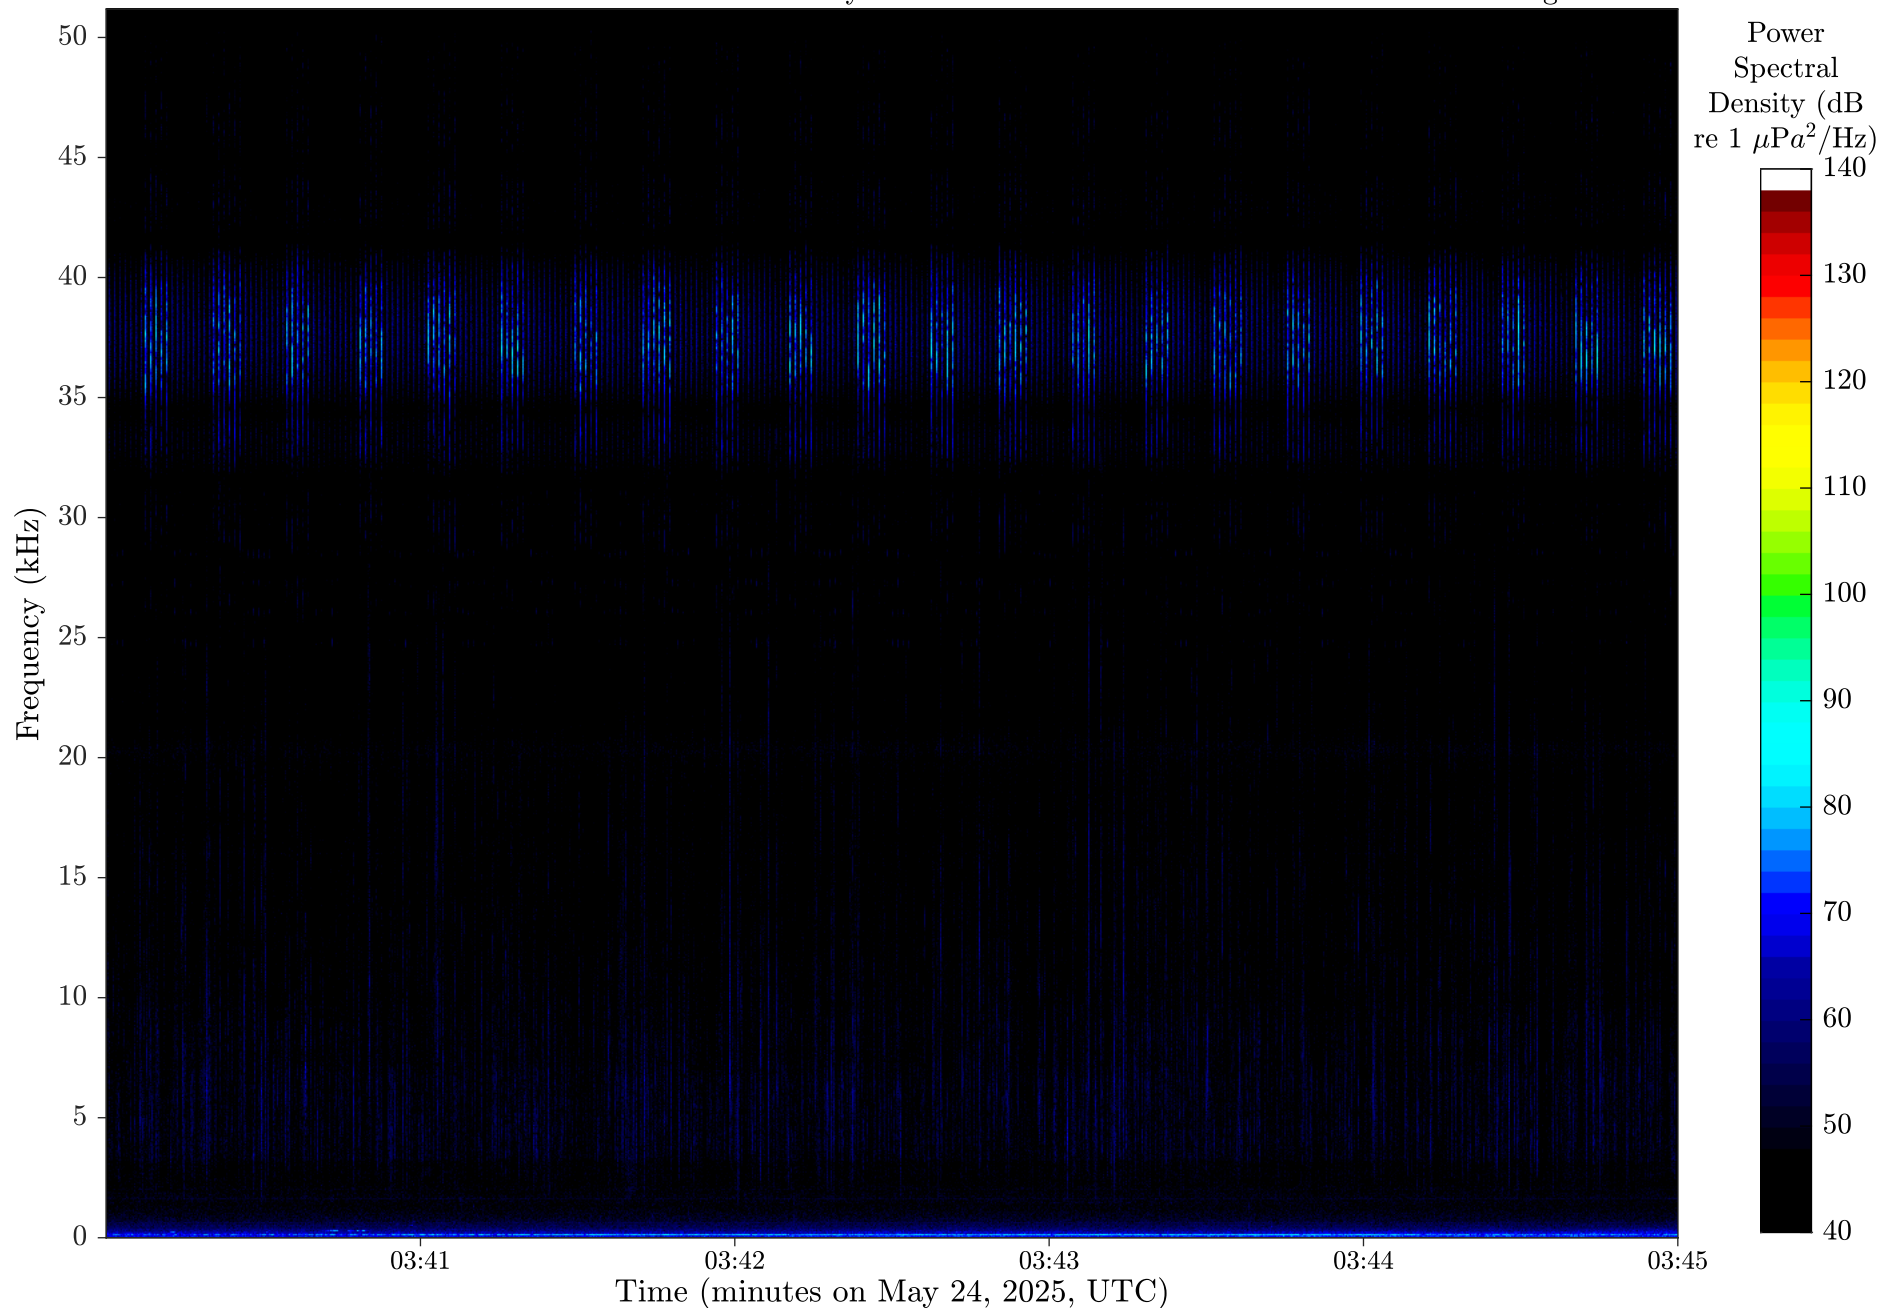

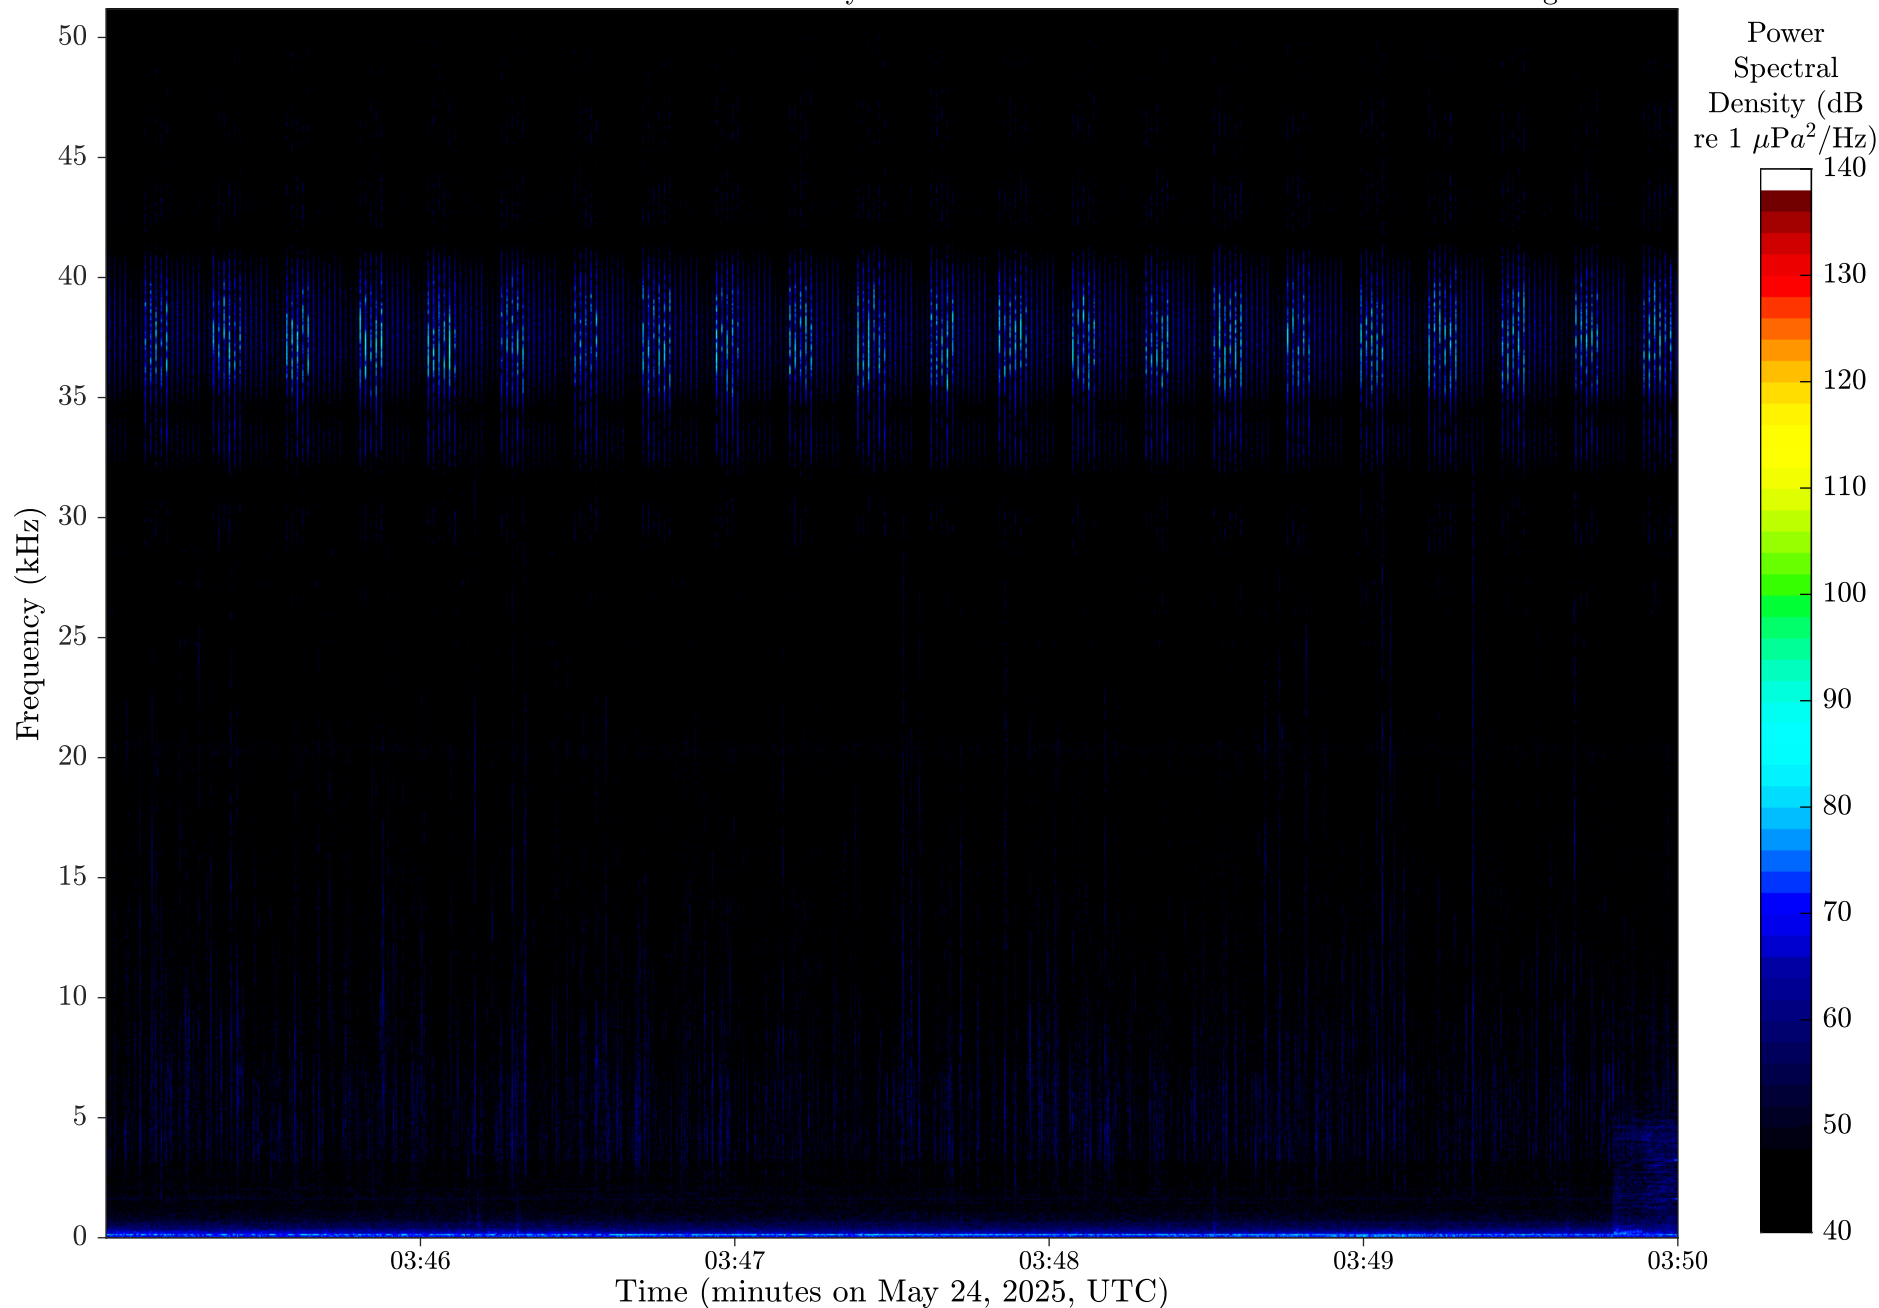


Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:13:46 UTC

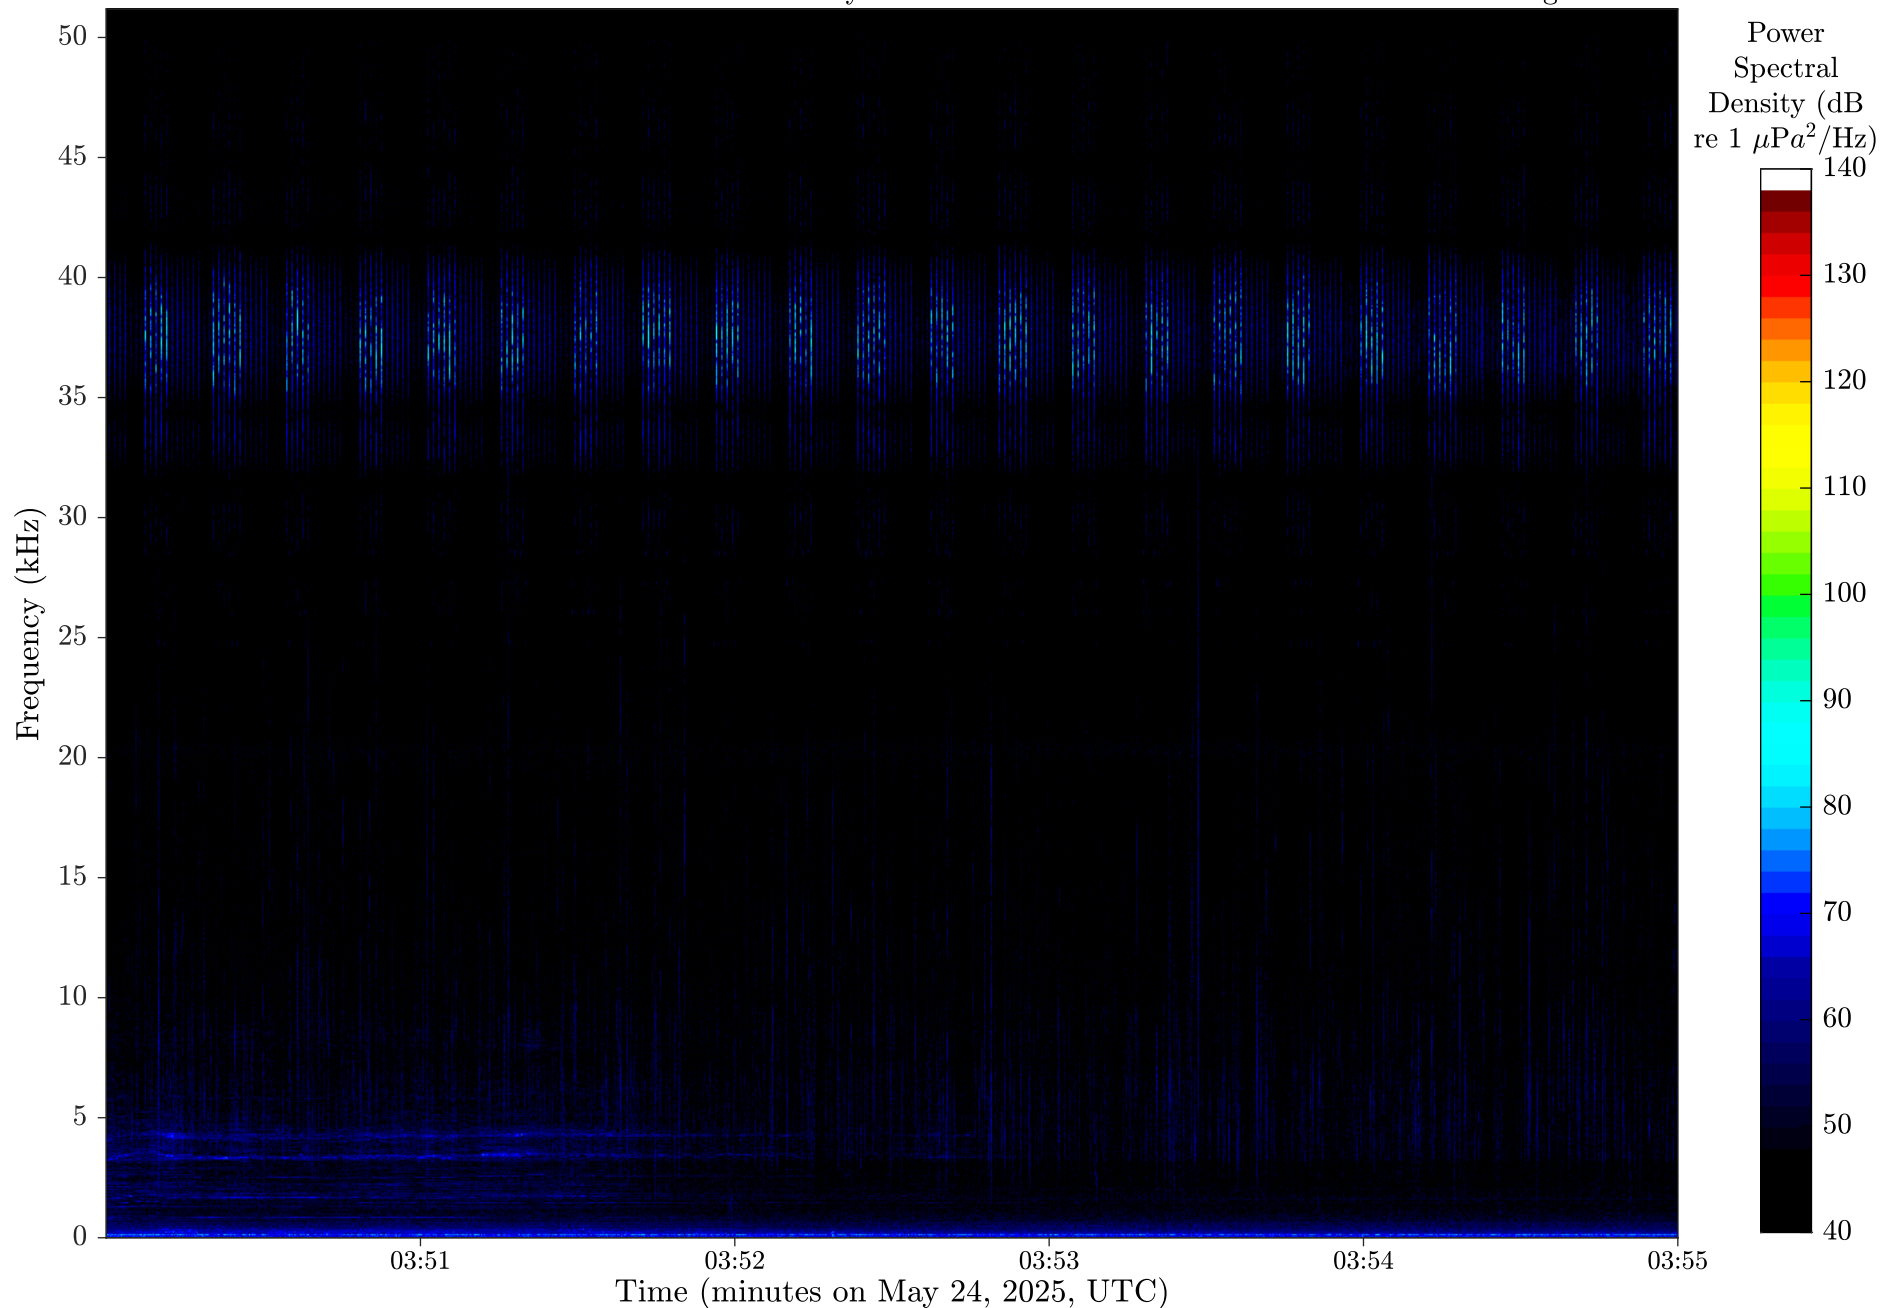


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:13:54 UTC

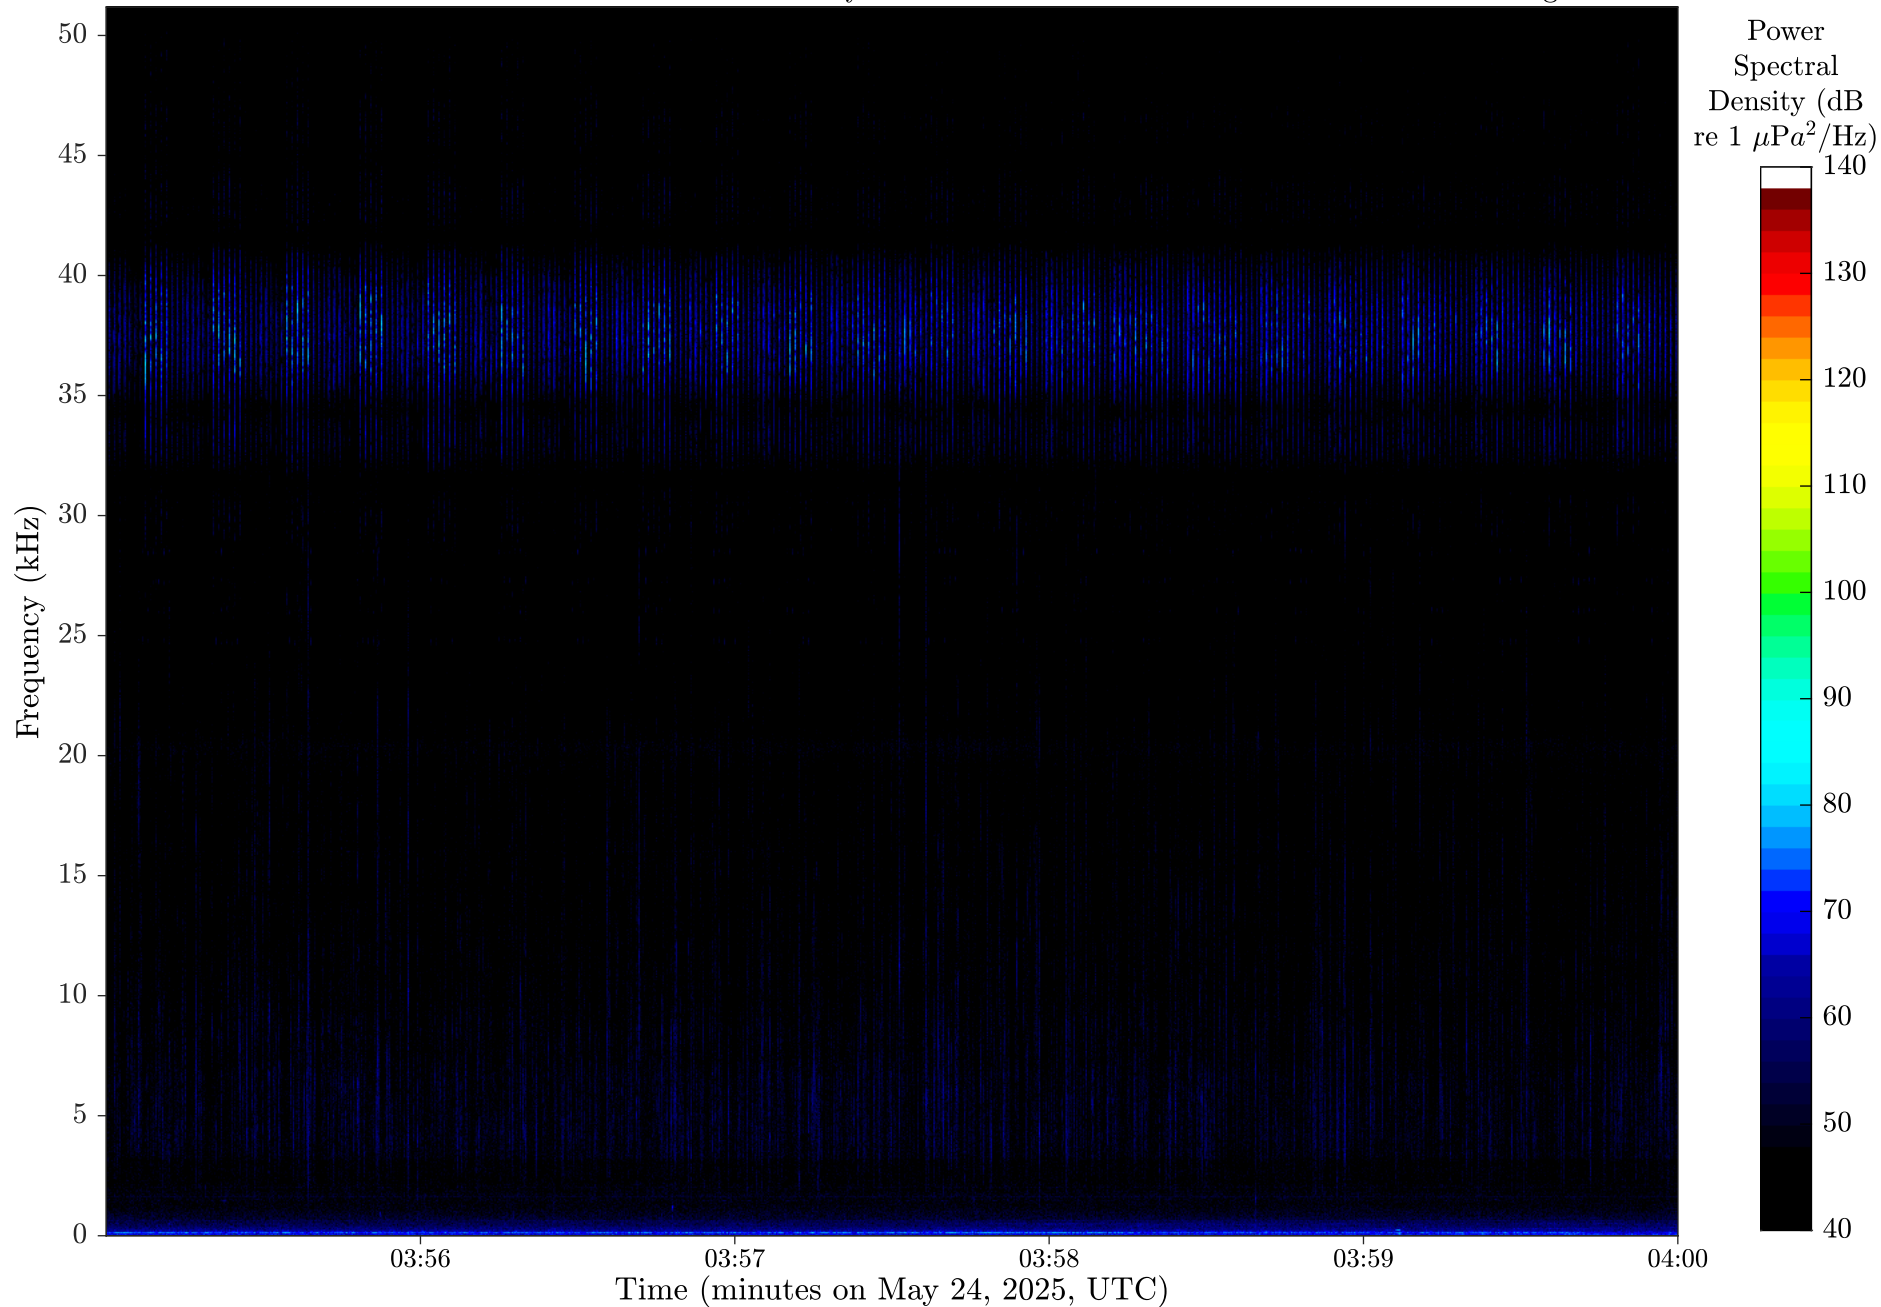


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:14:02 UTC

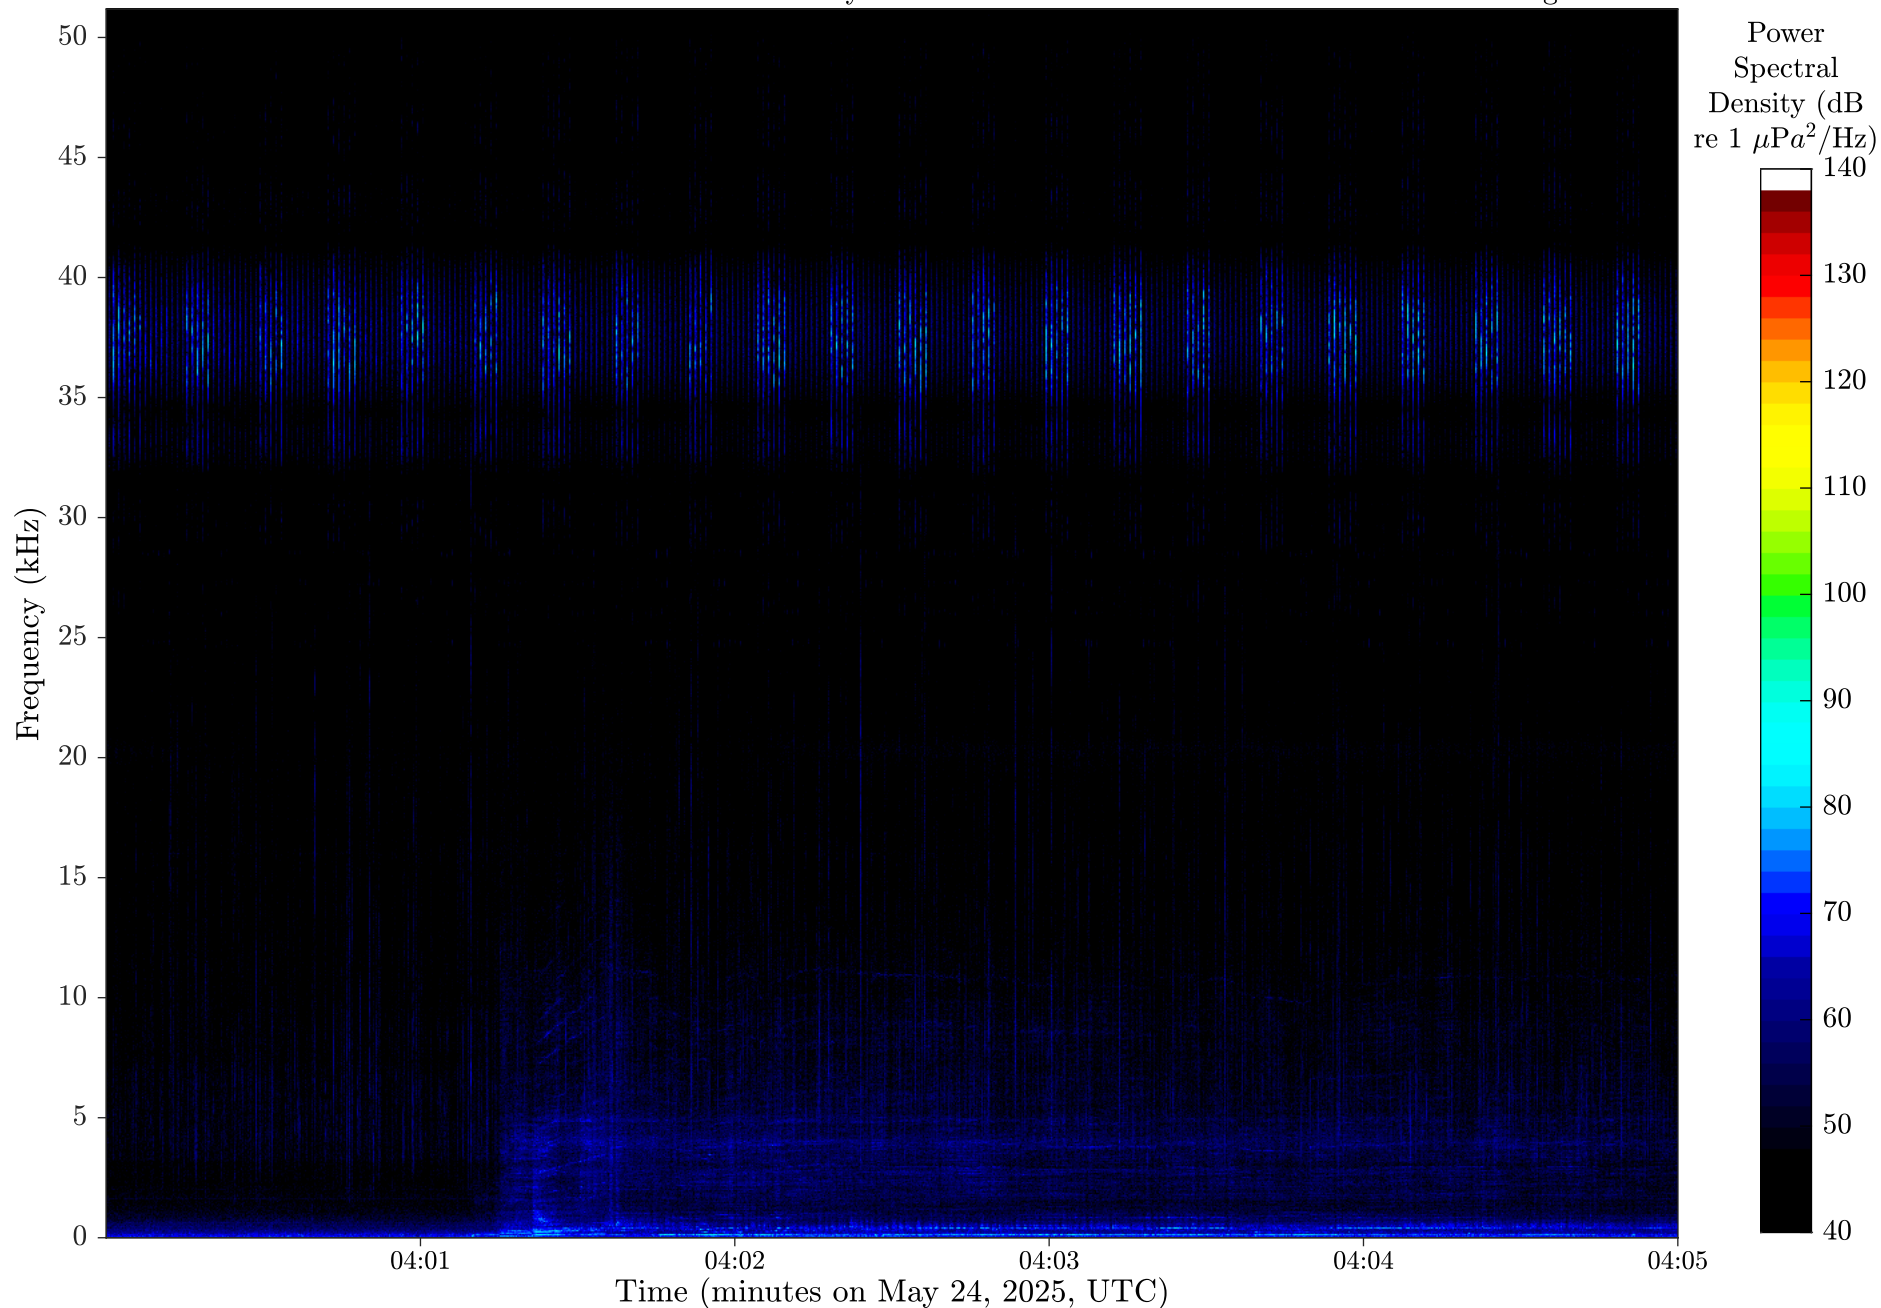


Comments: 32.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:14:09 UTC

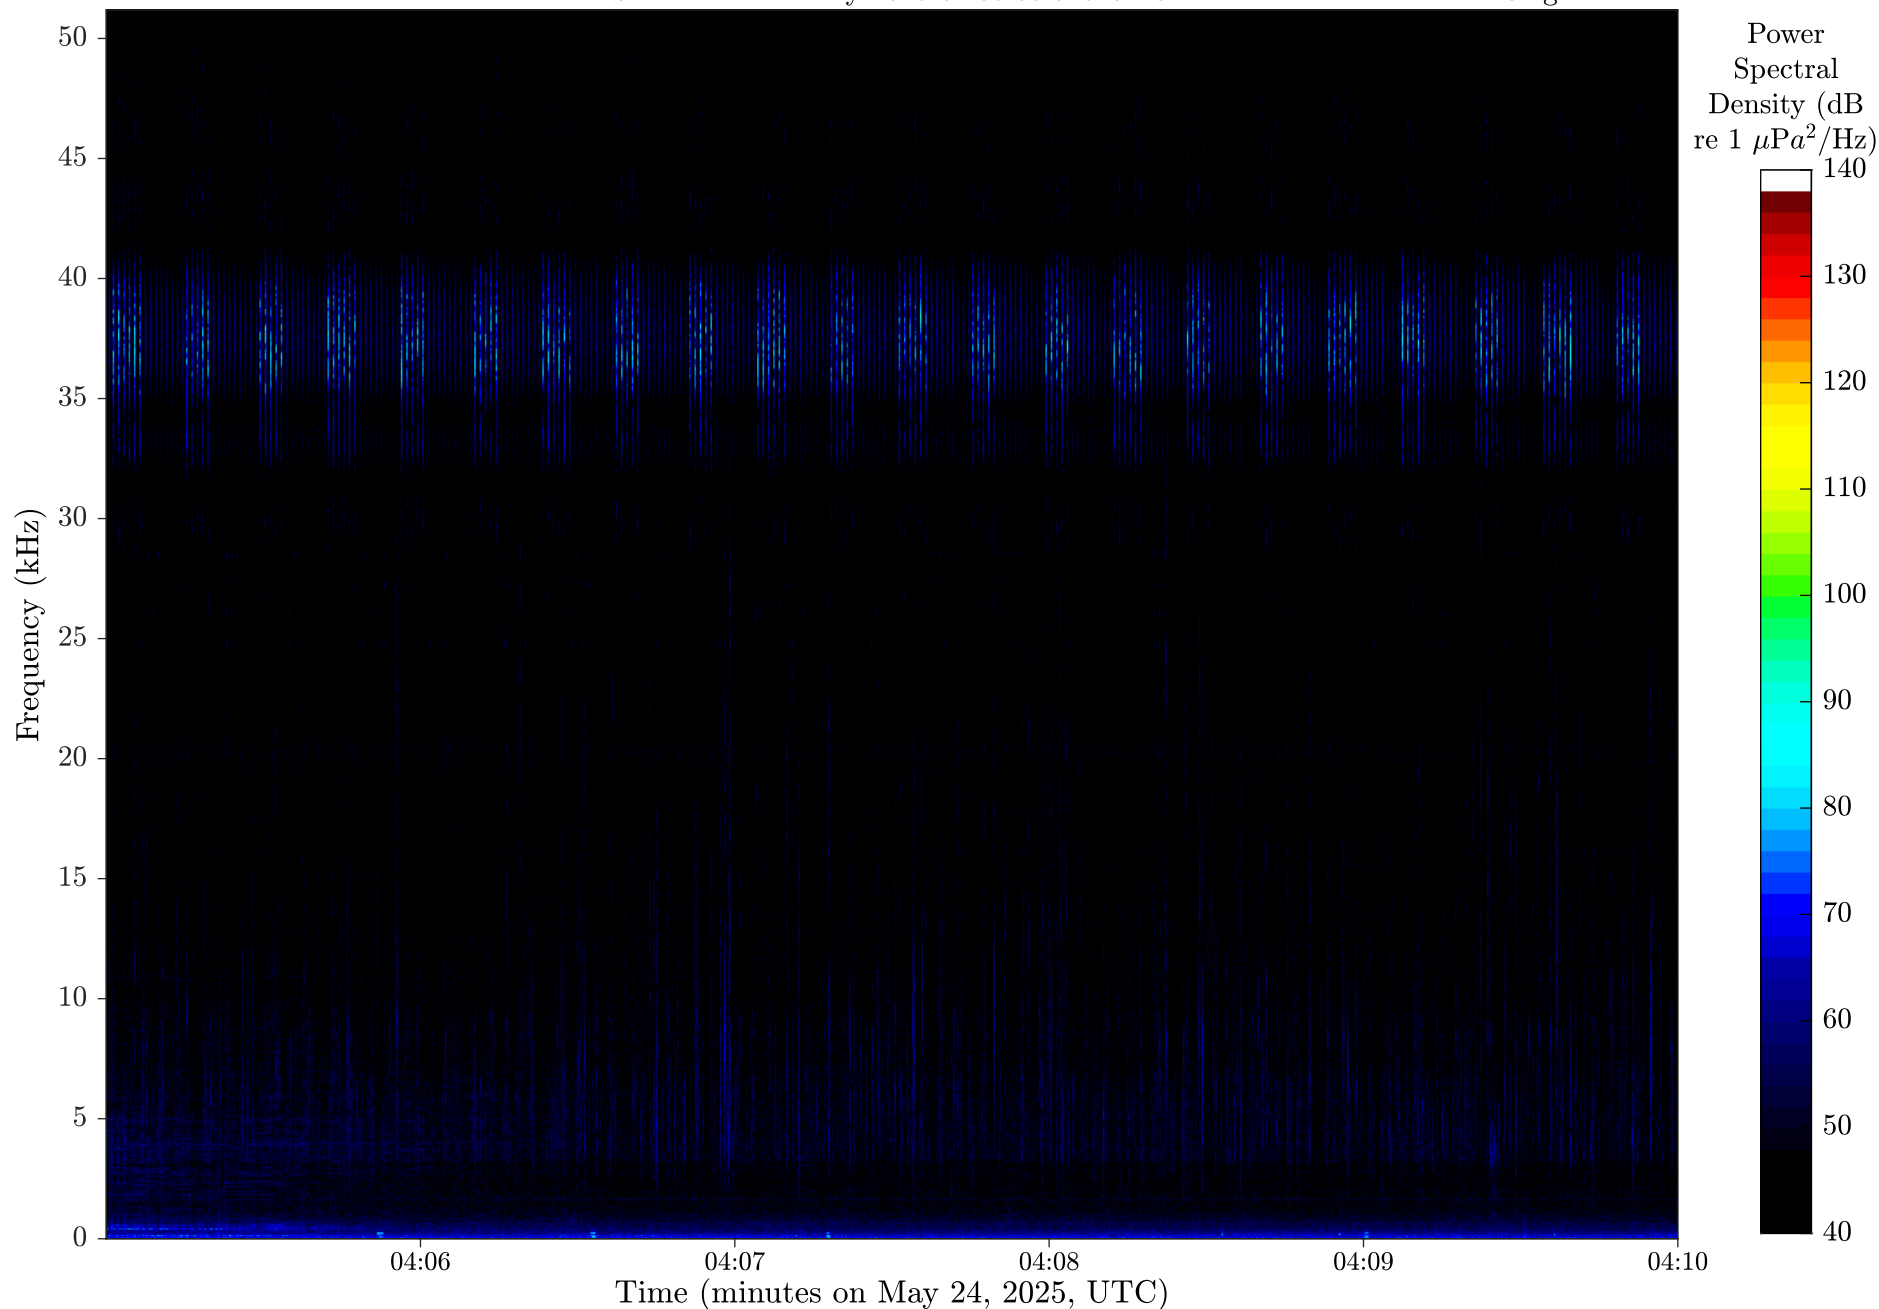


Comments: 34.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:14:17 UTC

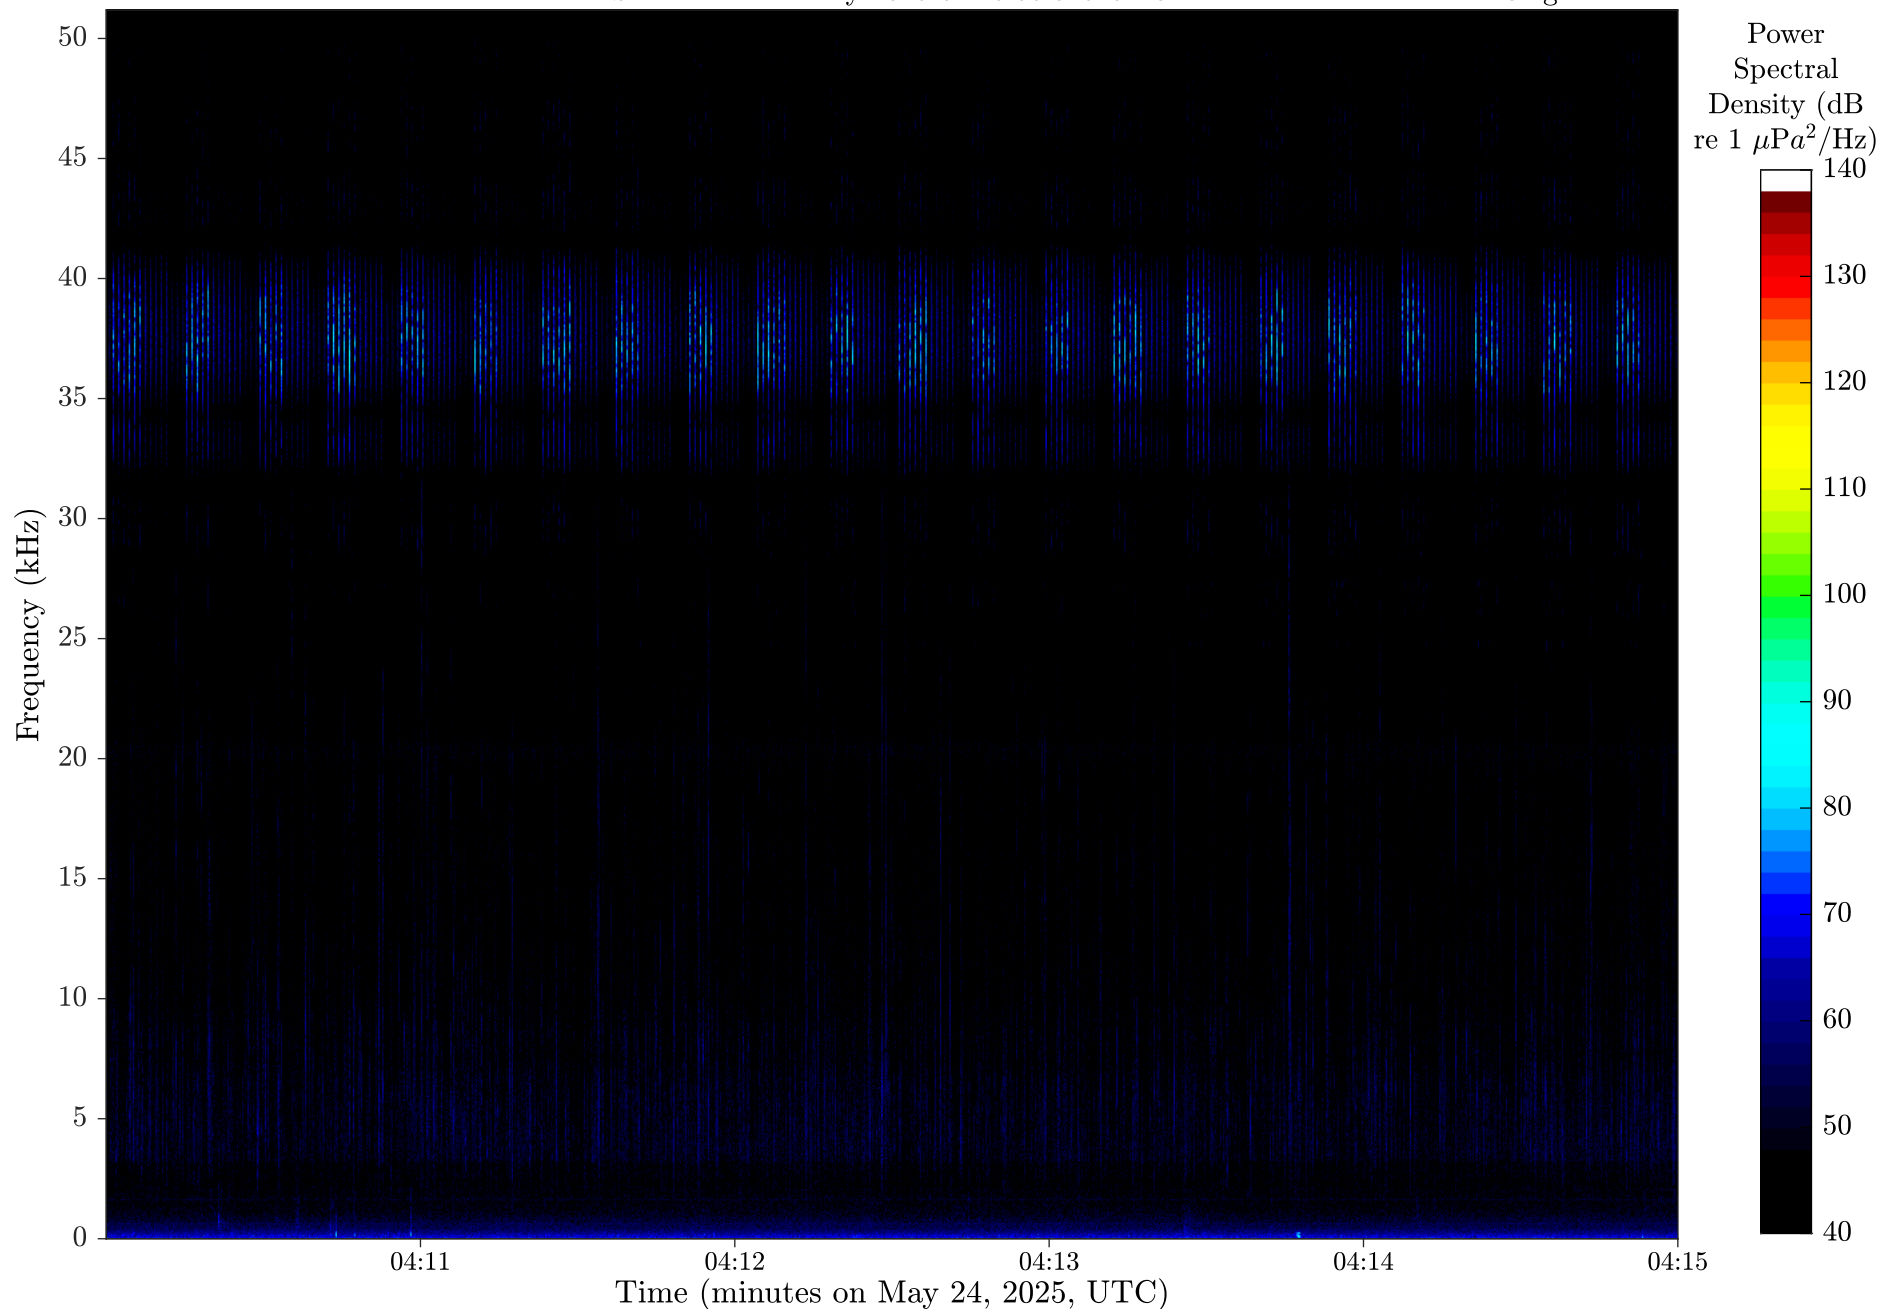



Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:14:24 UTC

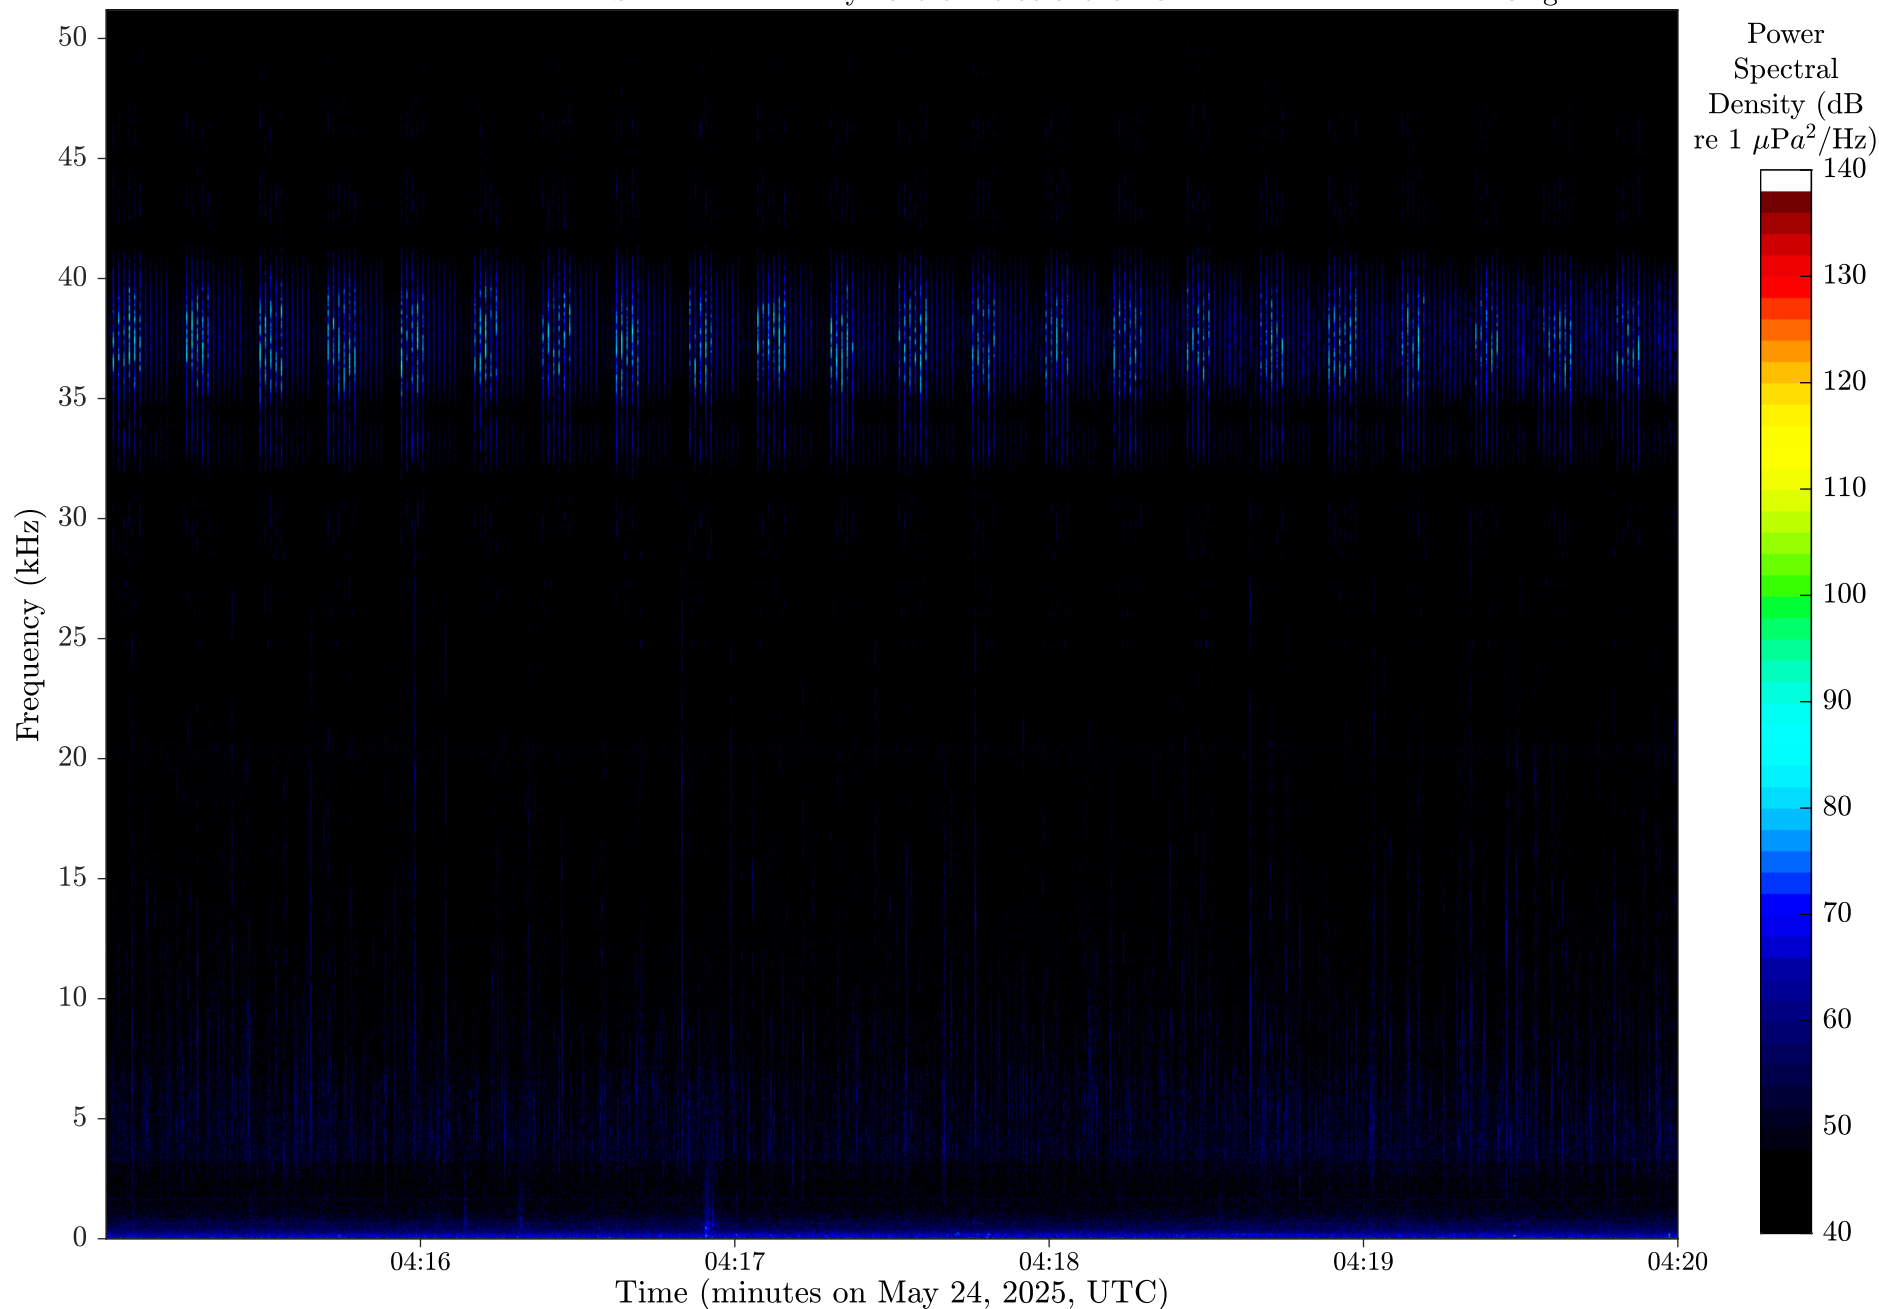

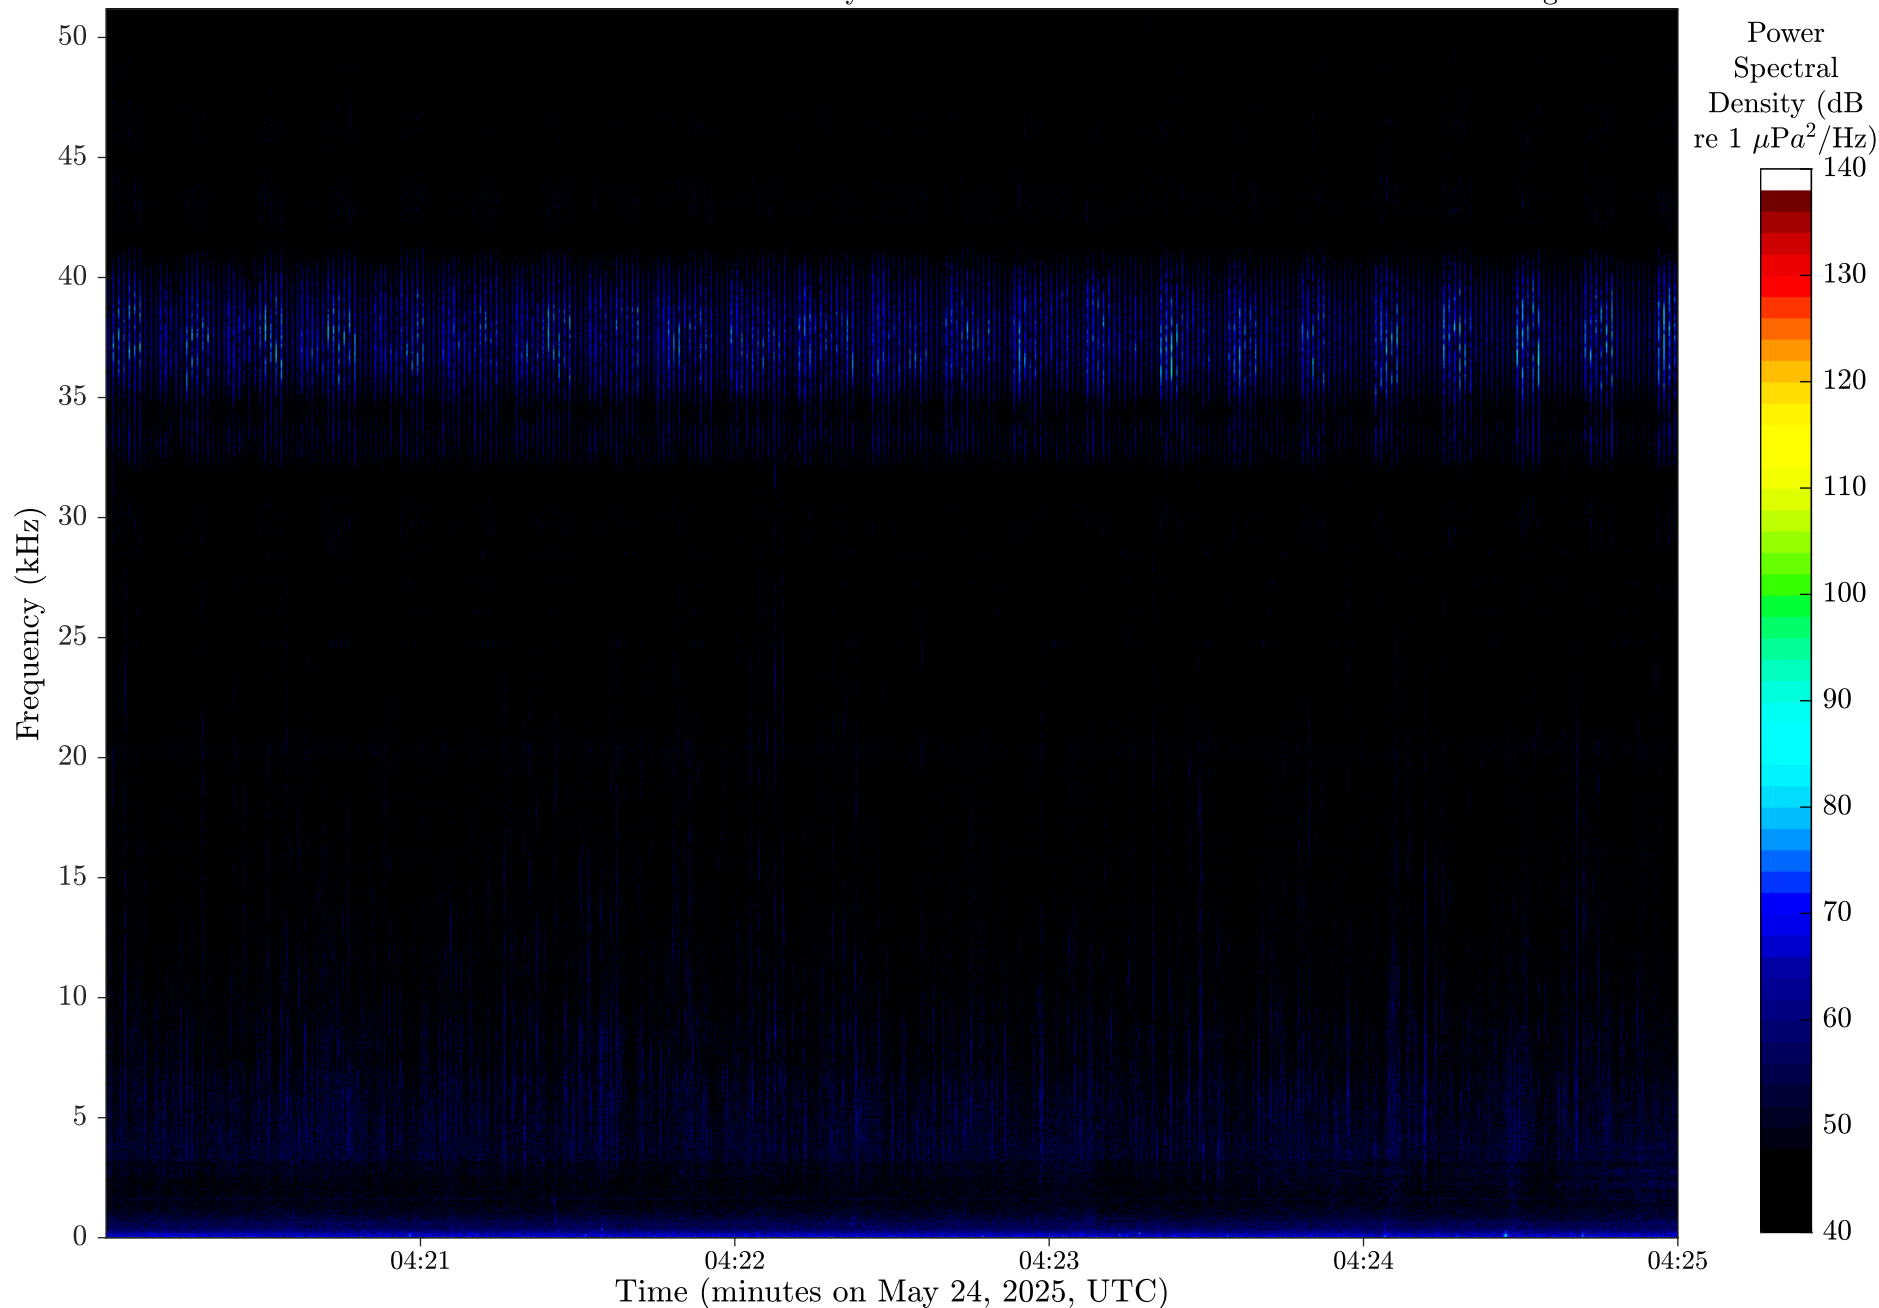


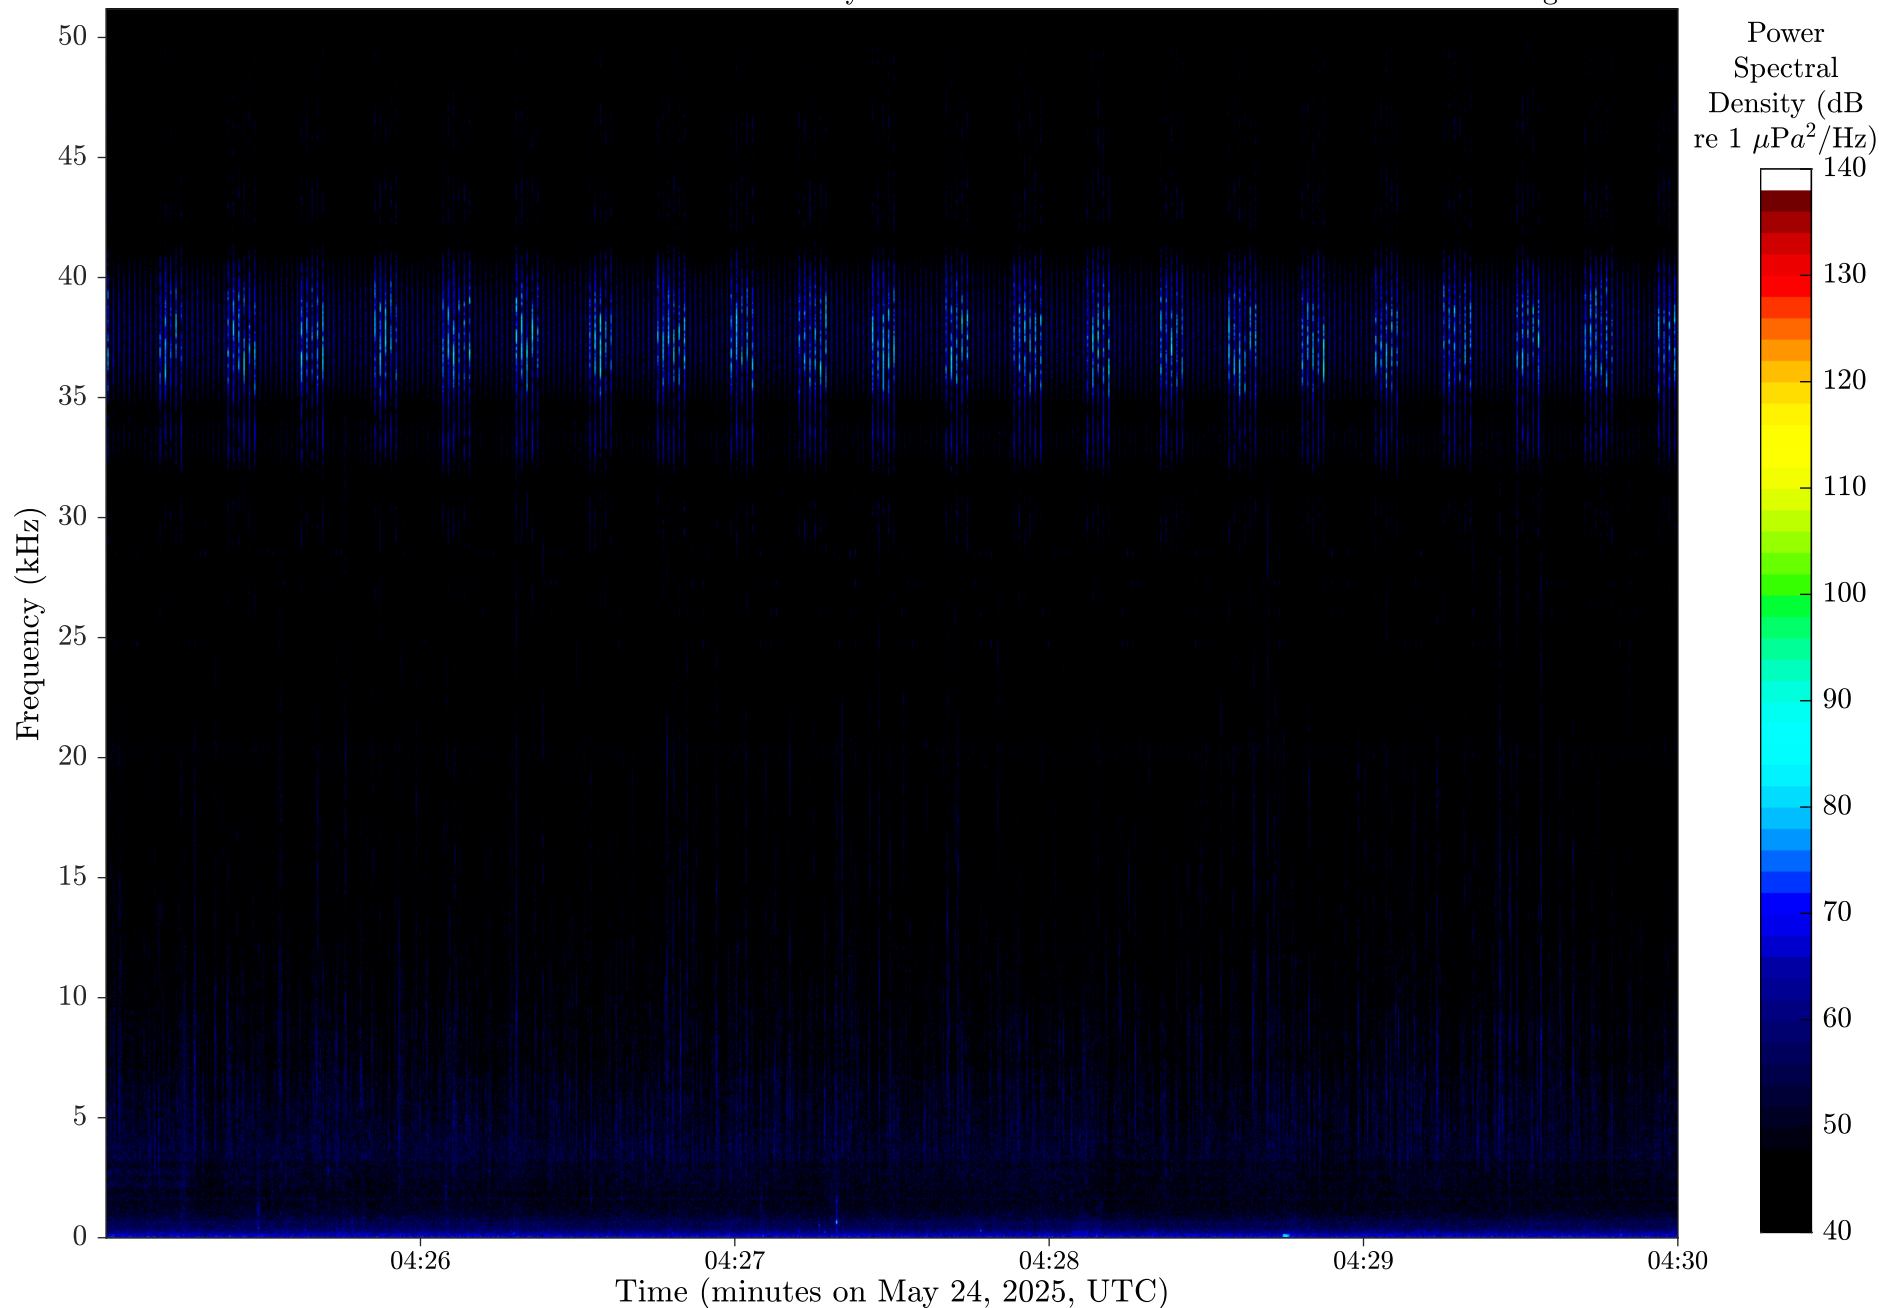

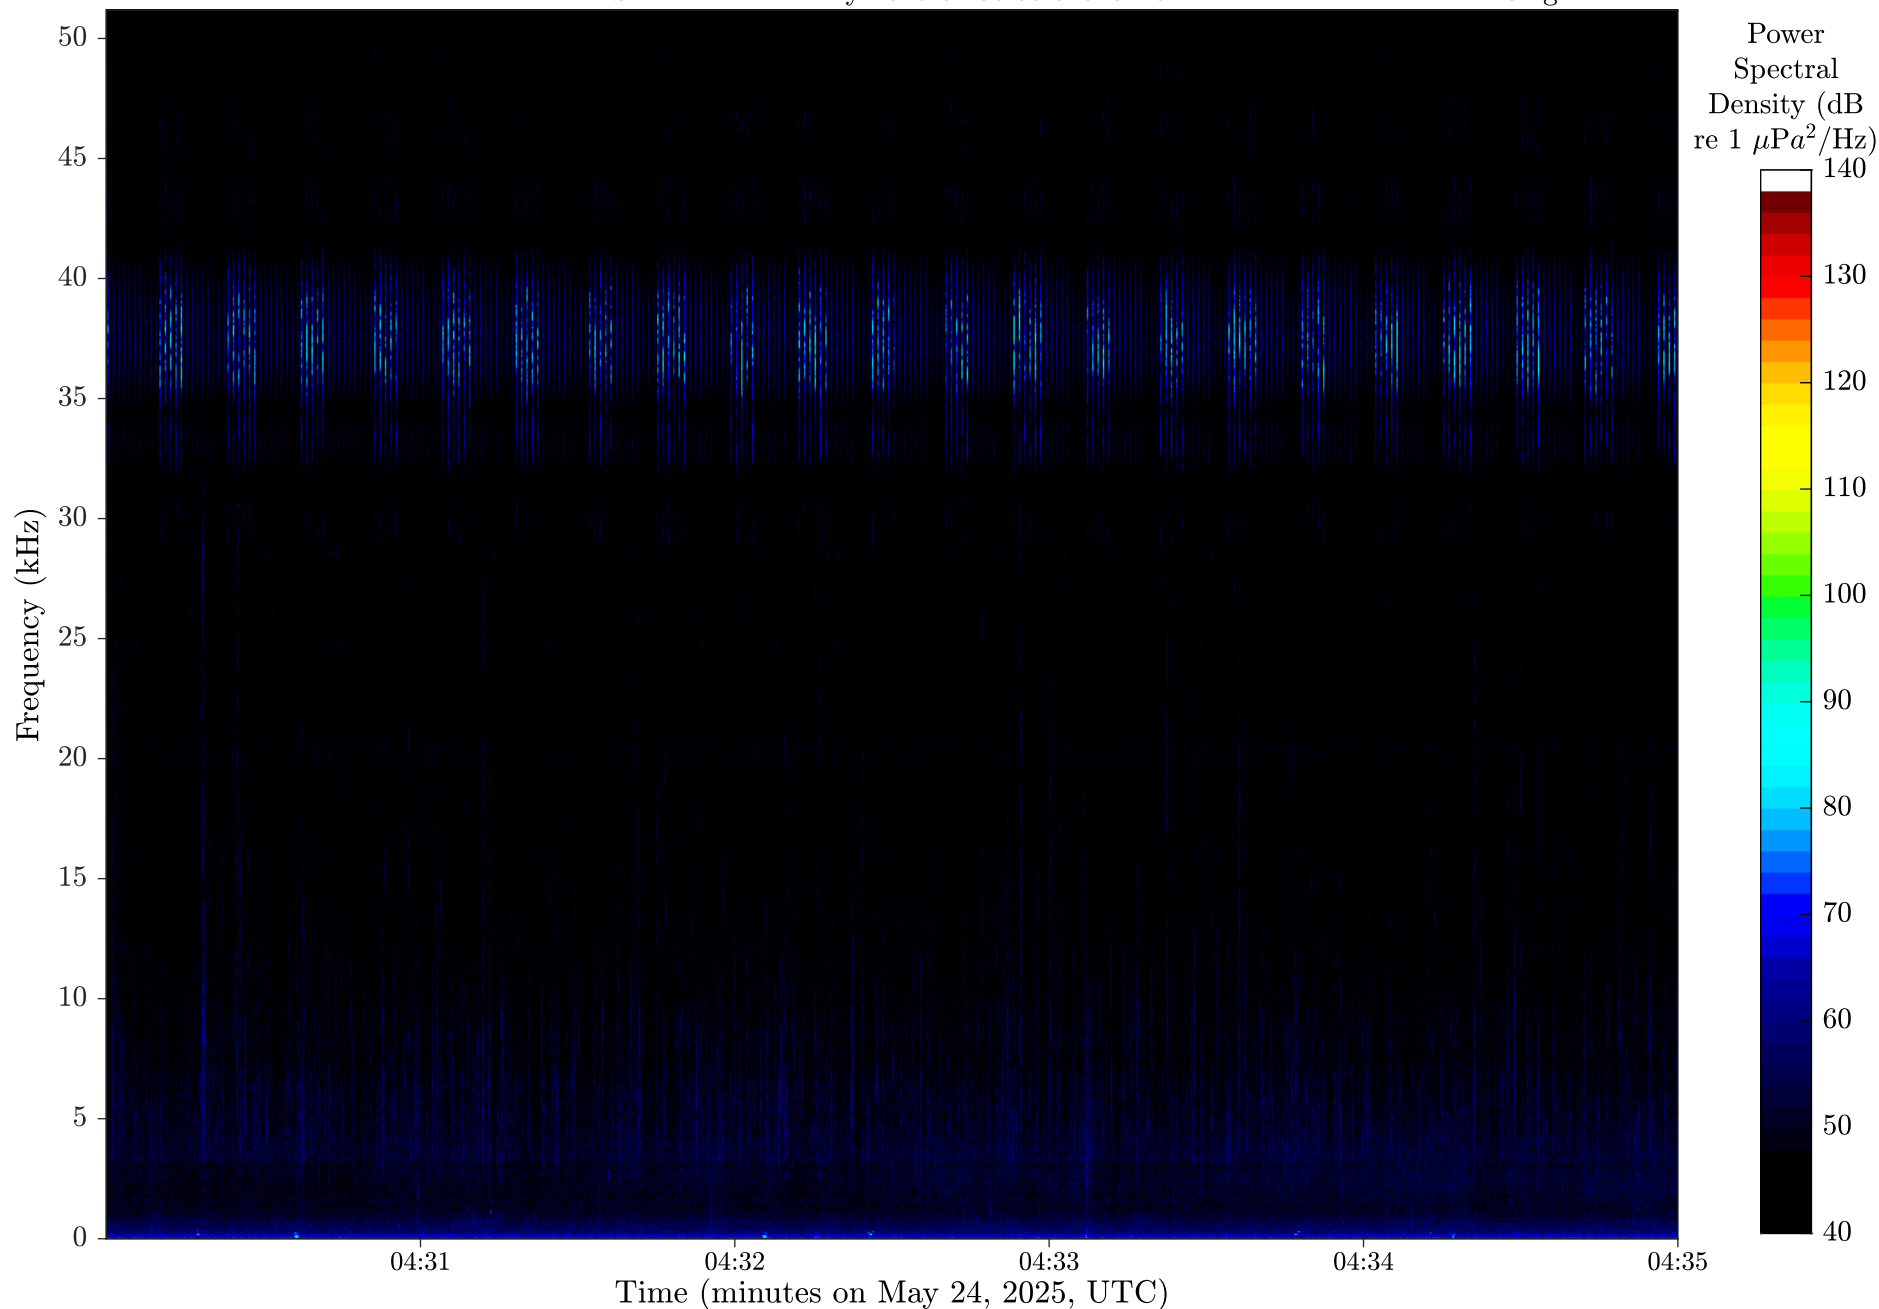


Comments: 34.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:14:54 UTC

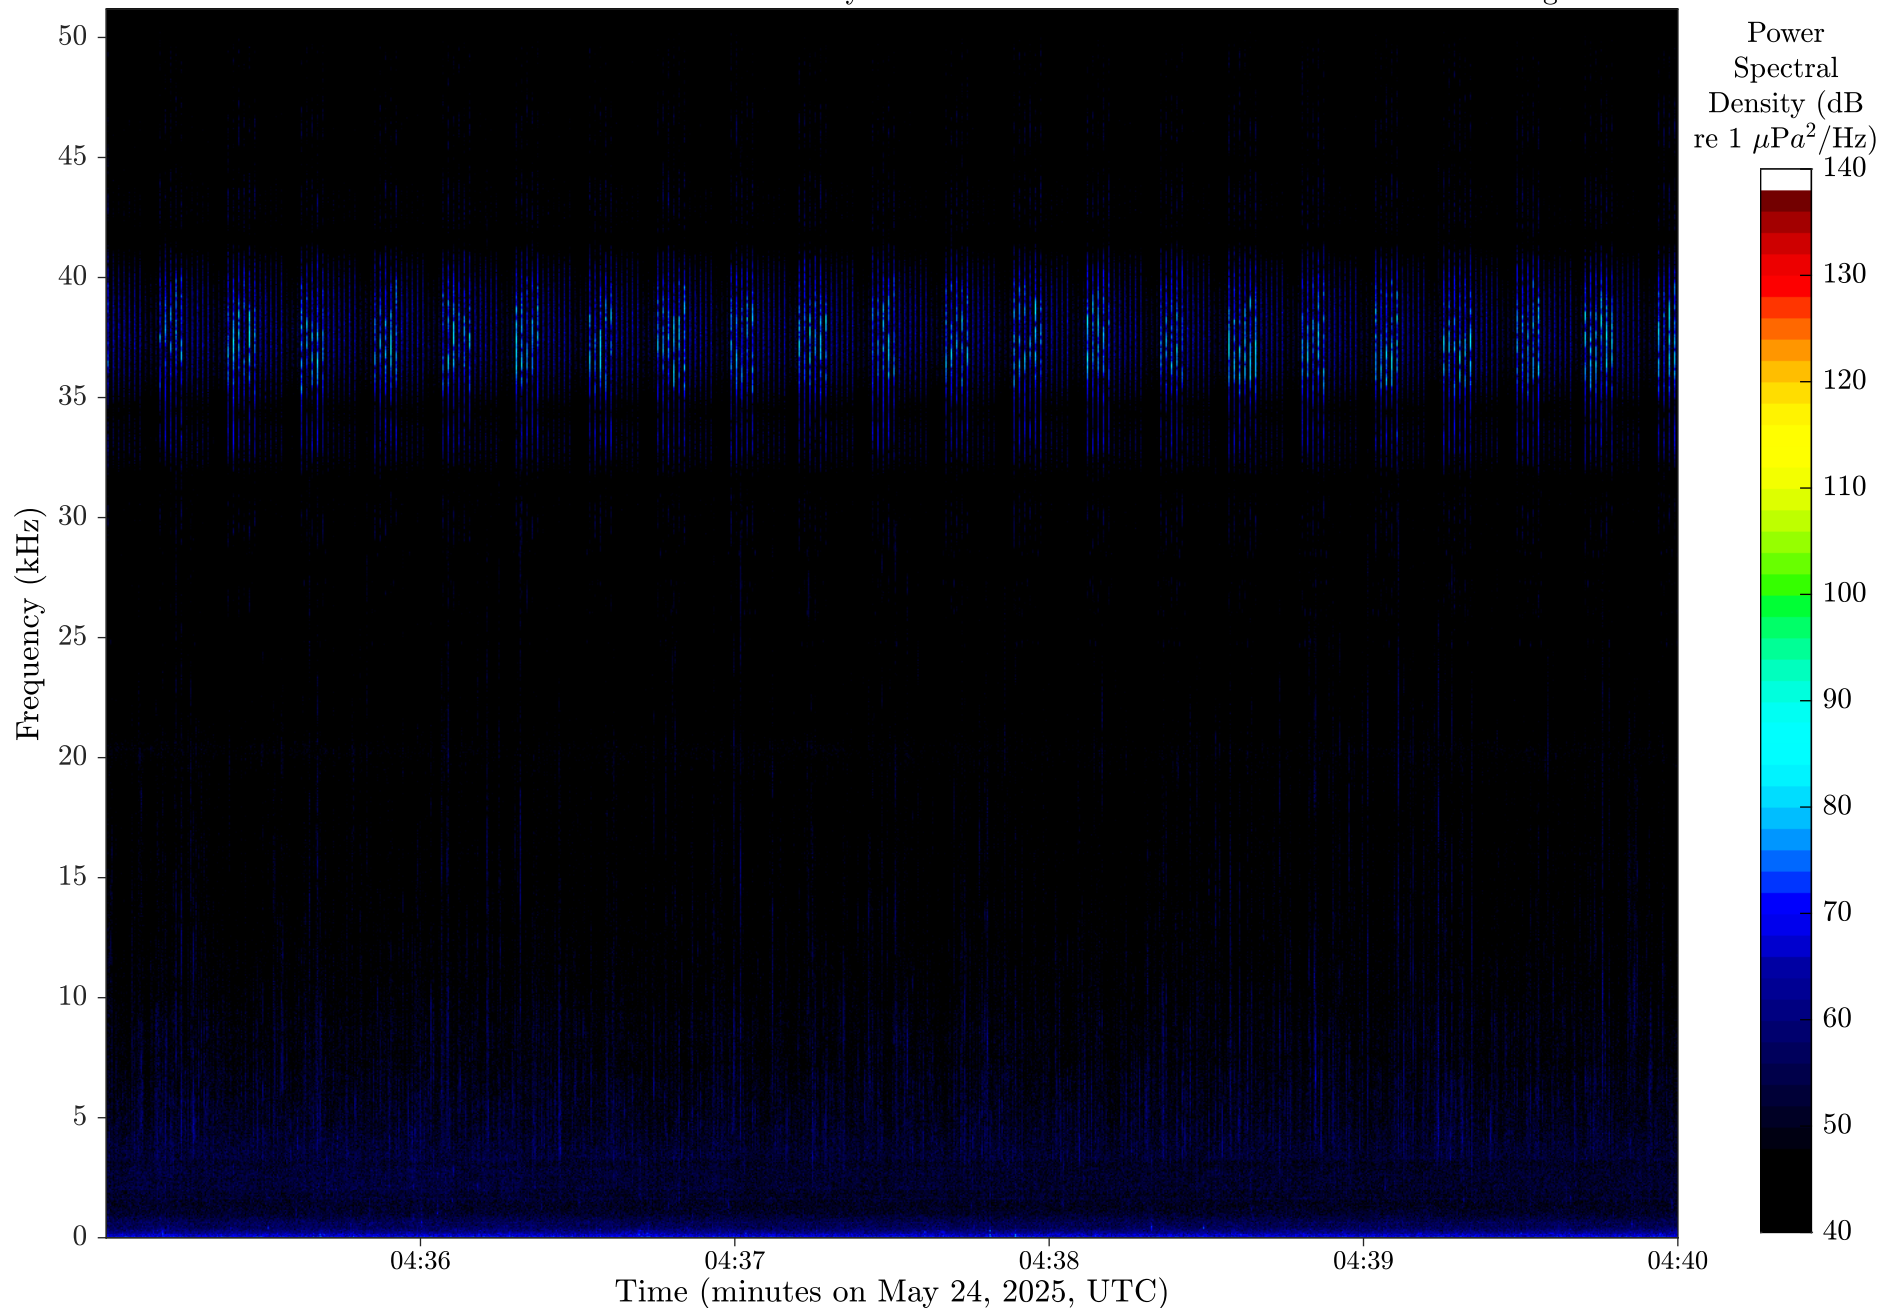


Comments: 34.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:15:02 UTC

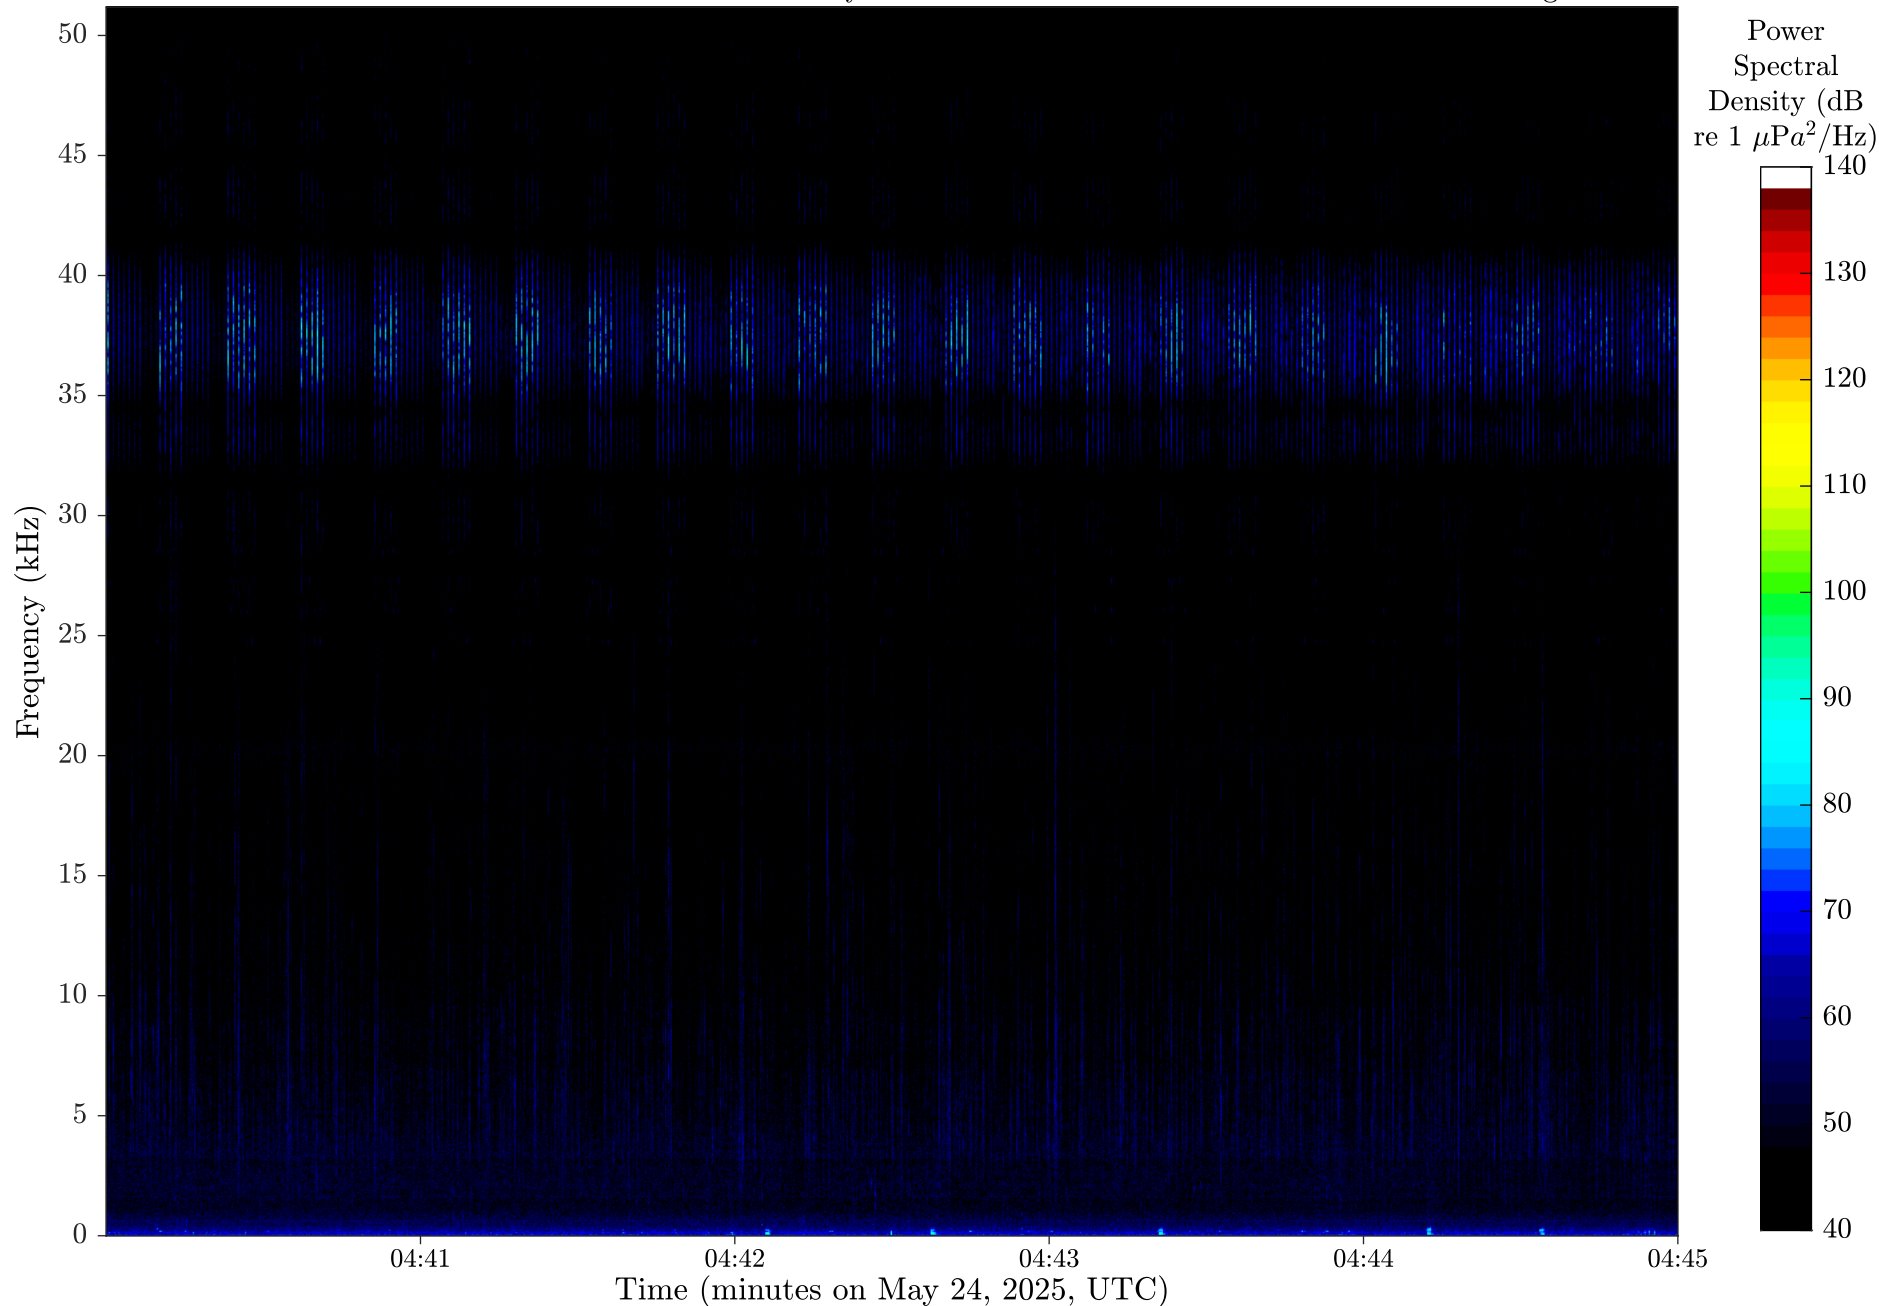

Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:15:10 UTC

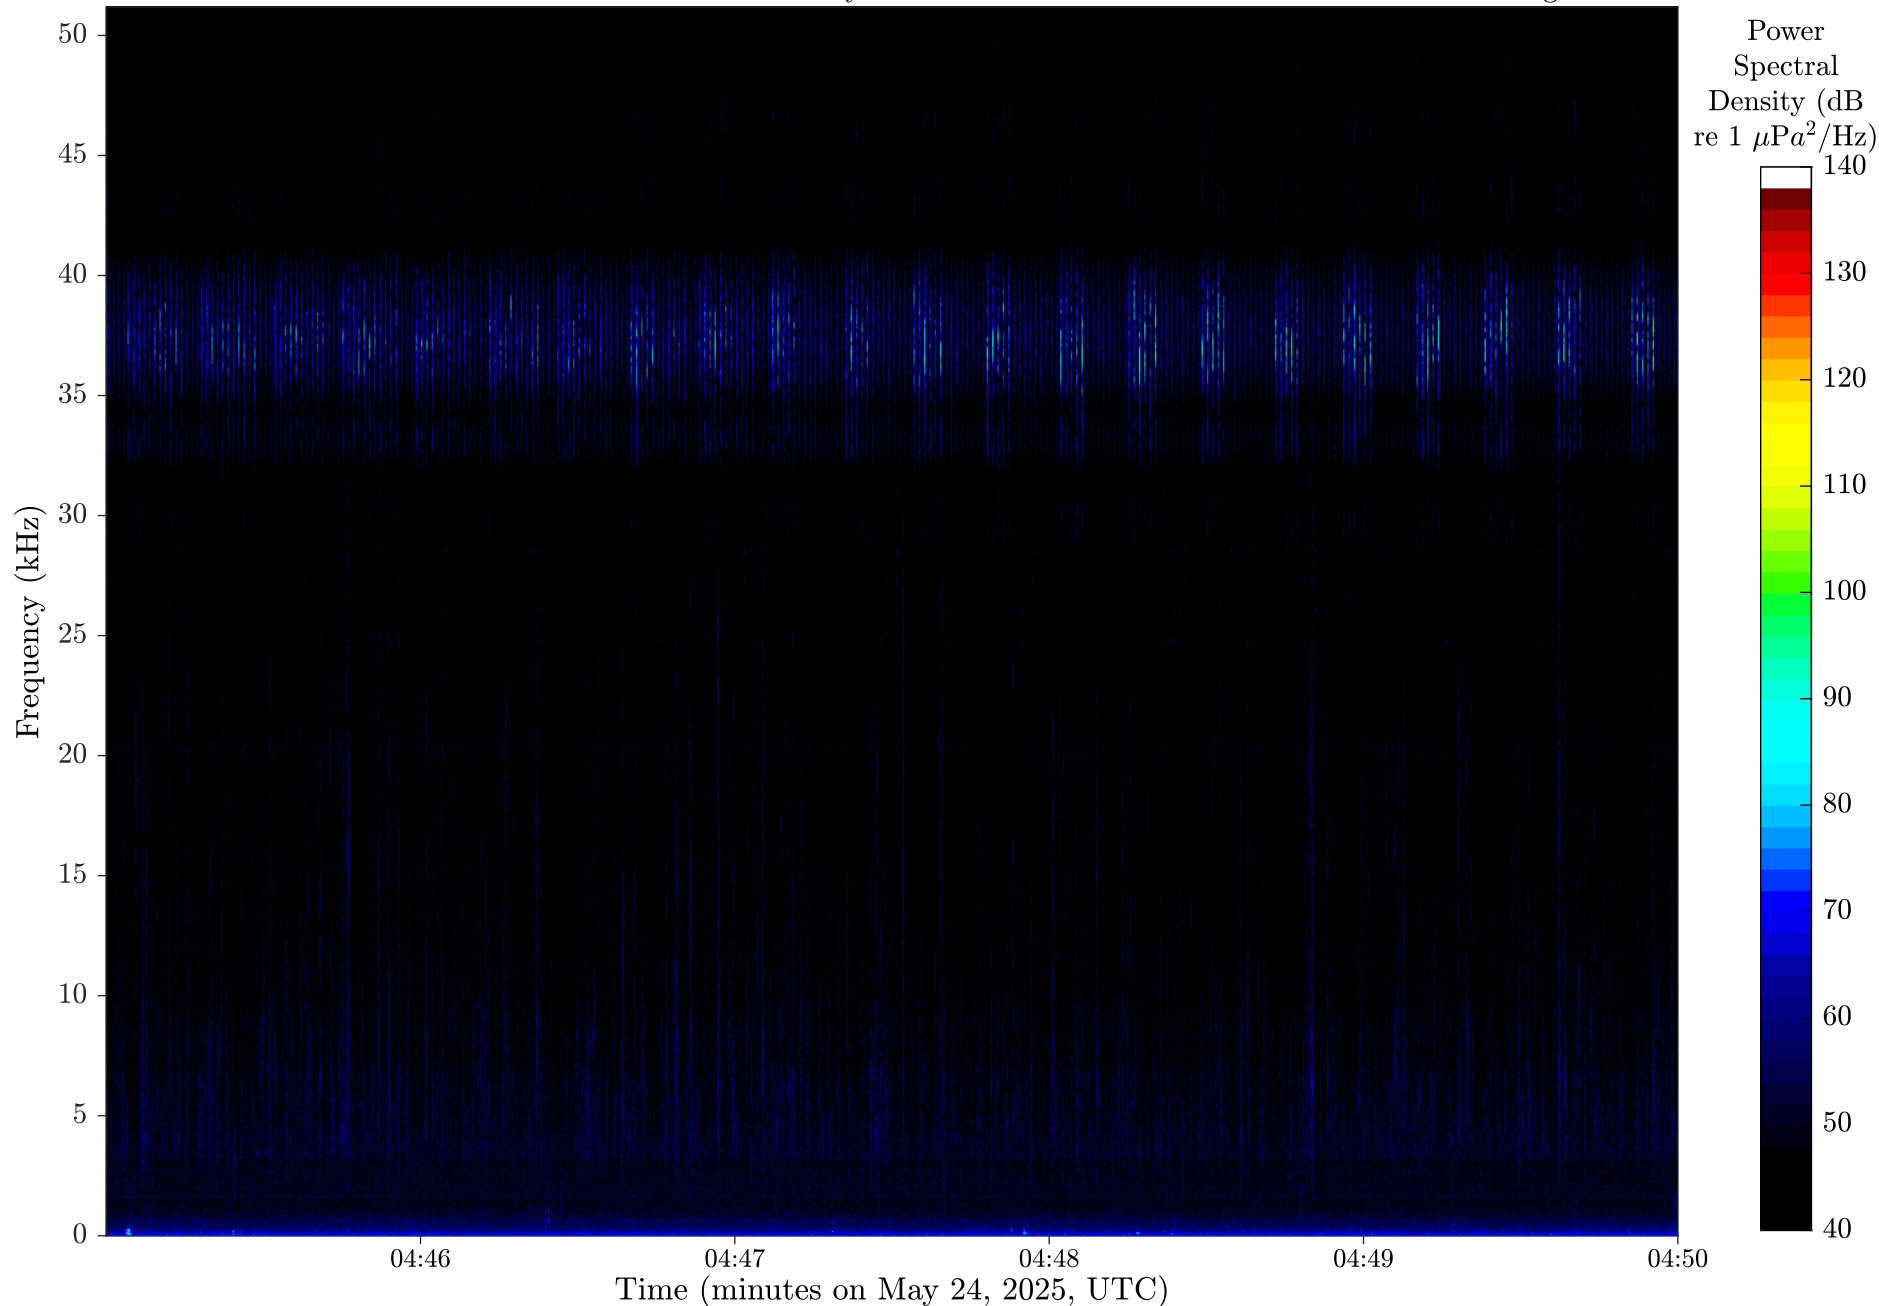

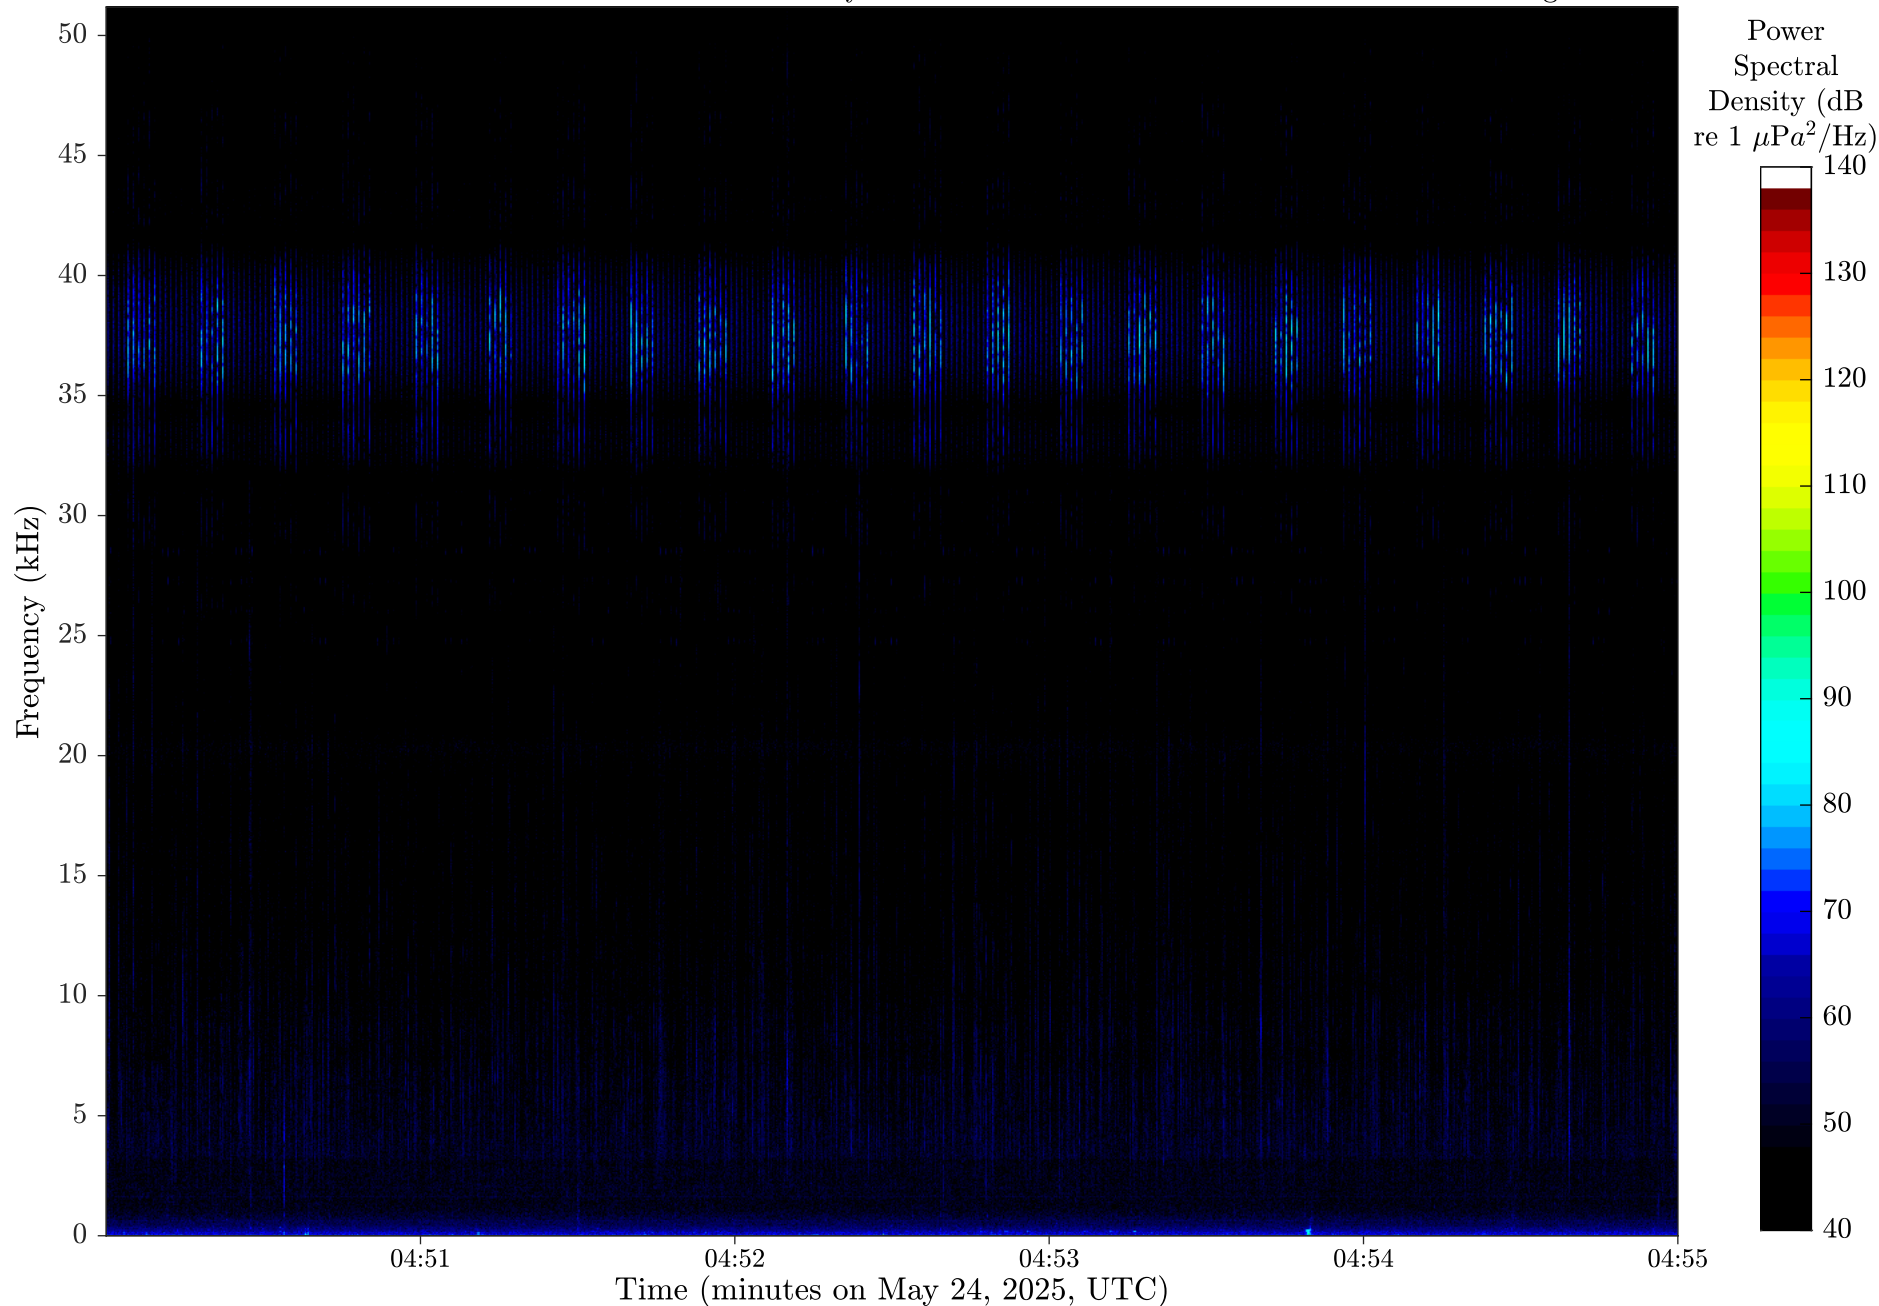


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:15:26 UTC

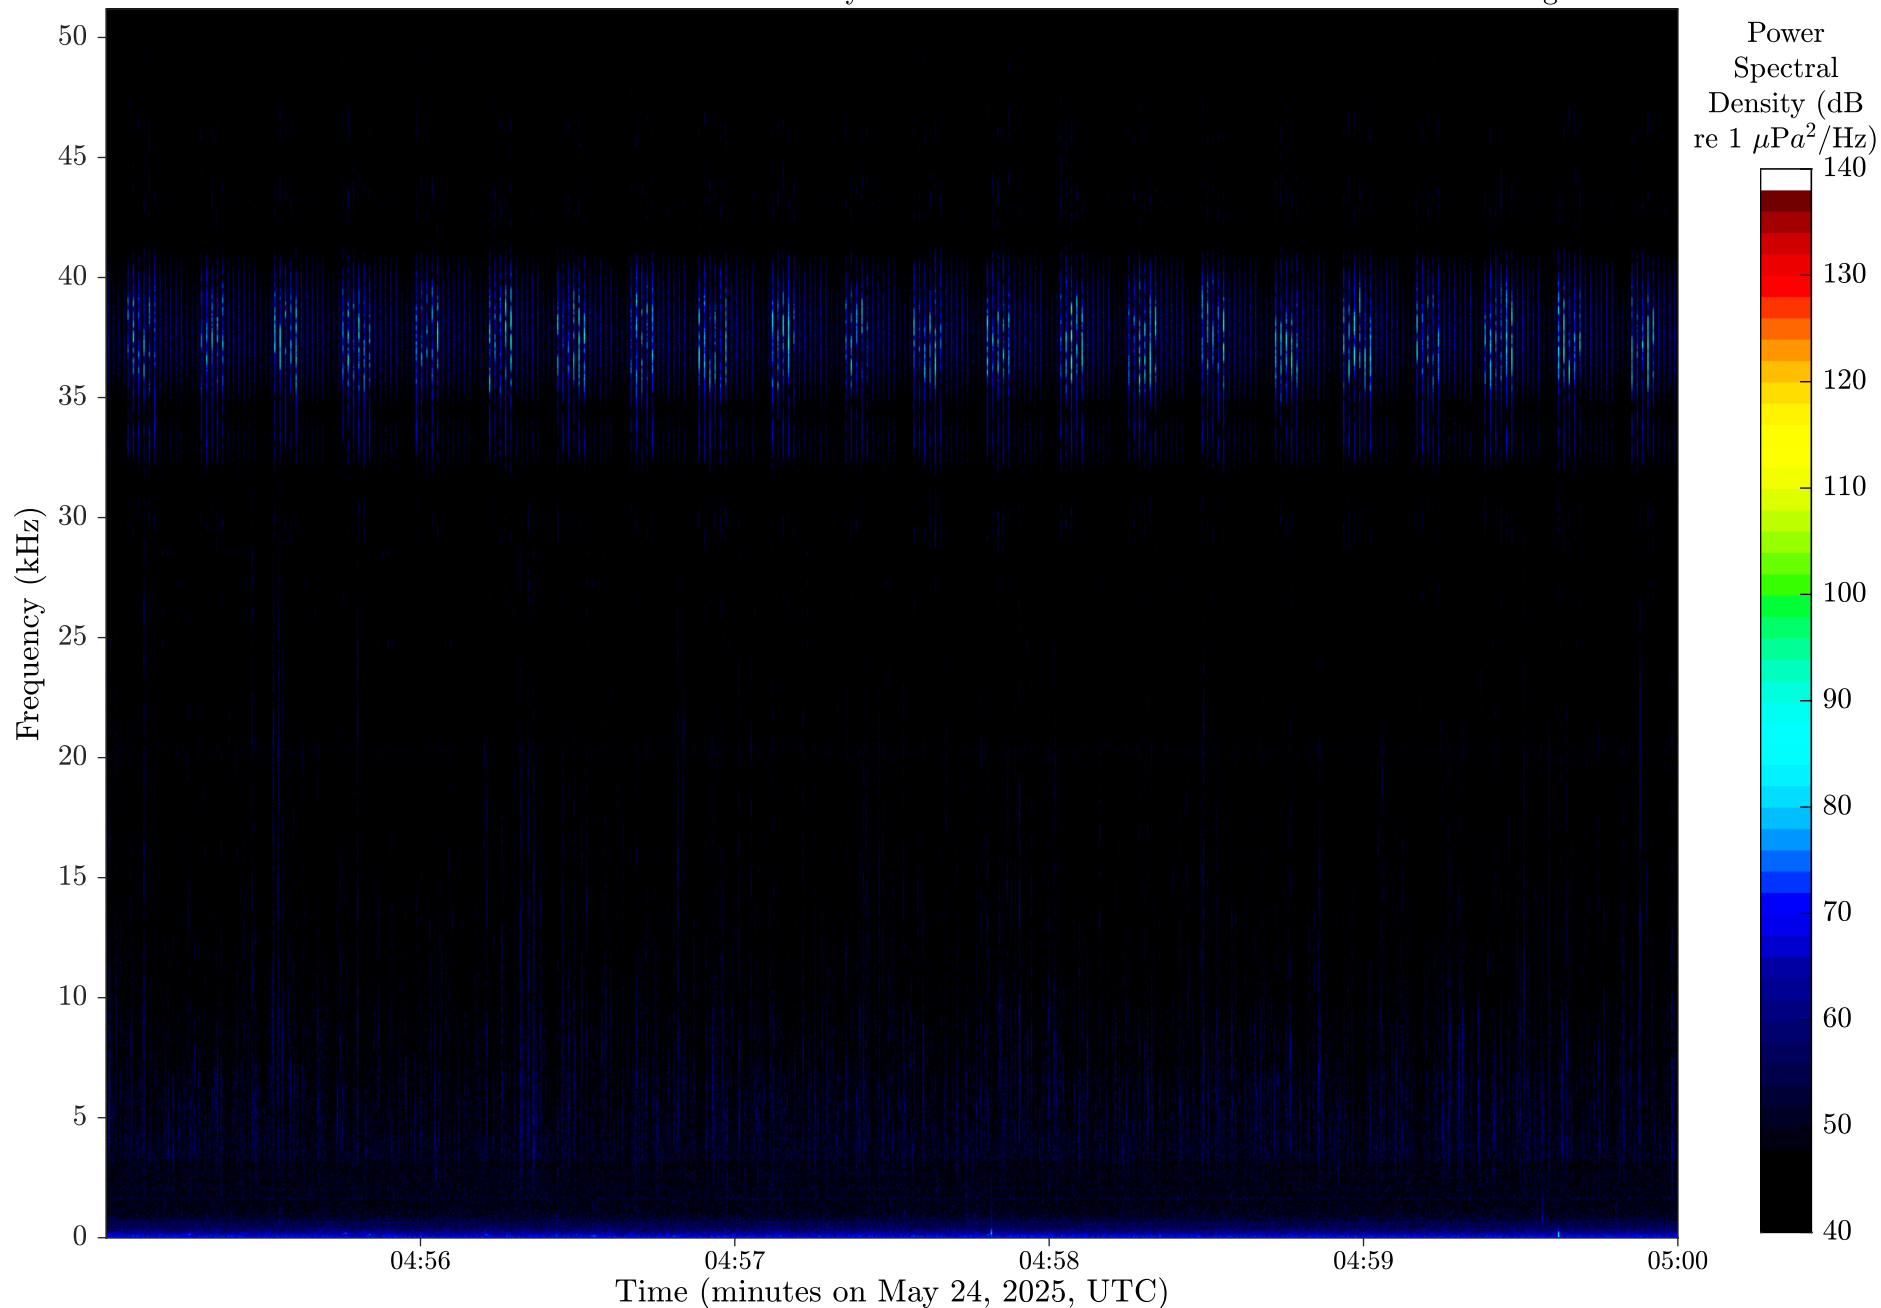



Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:15:33 UTC

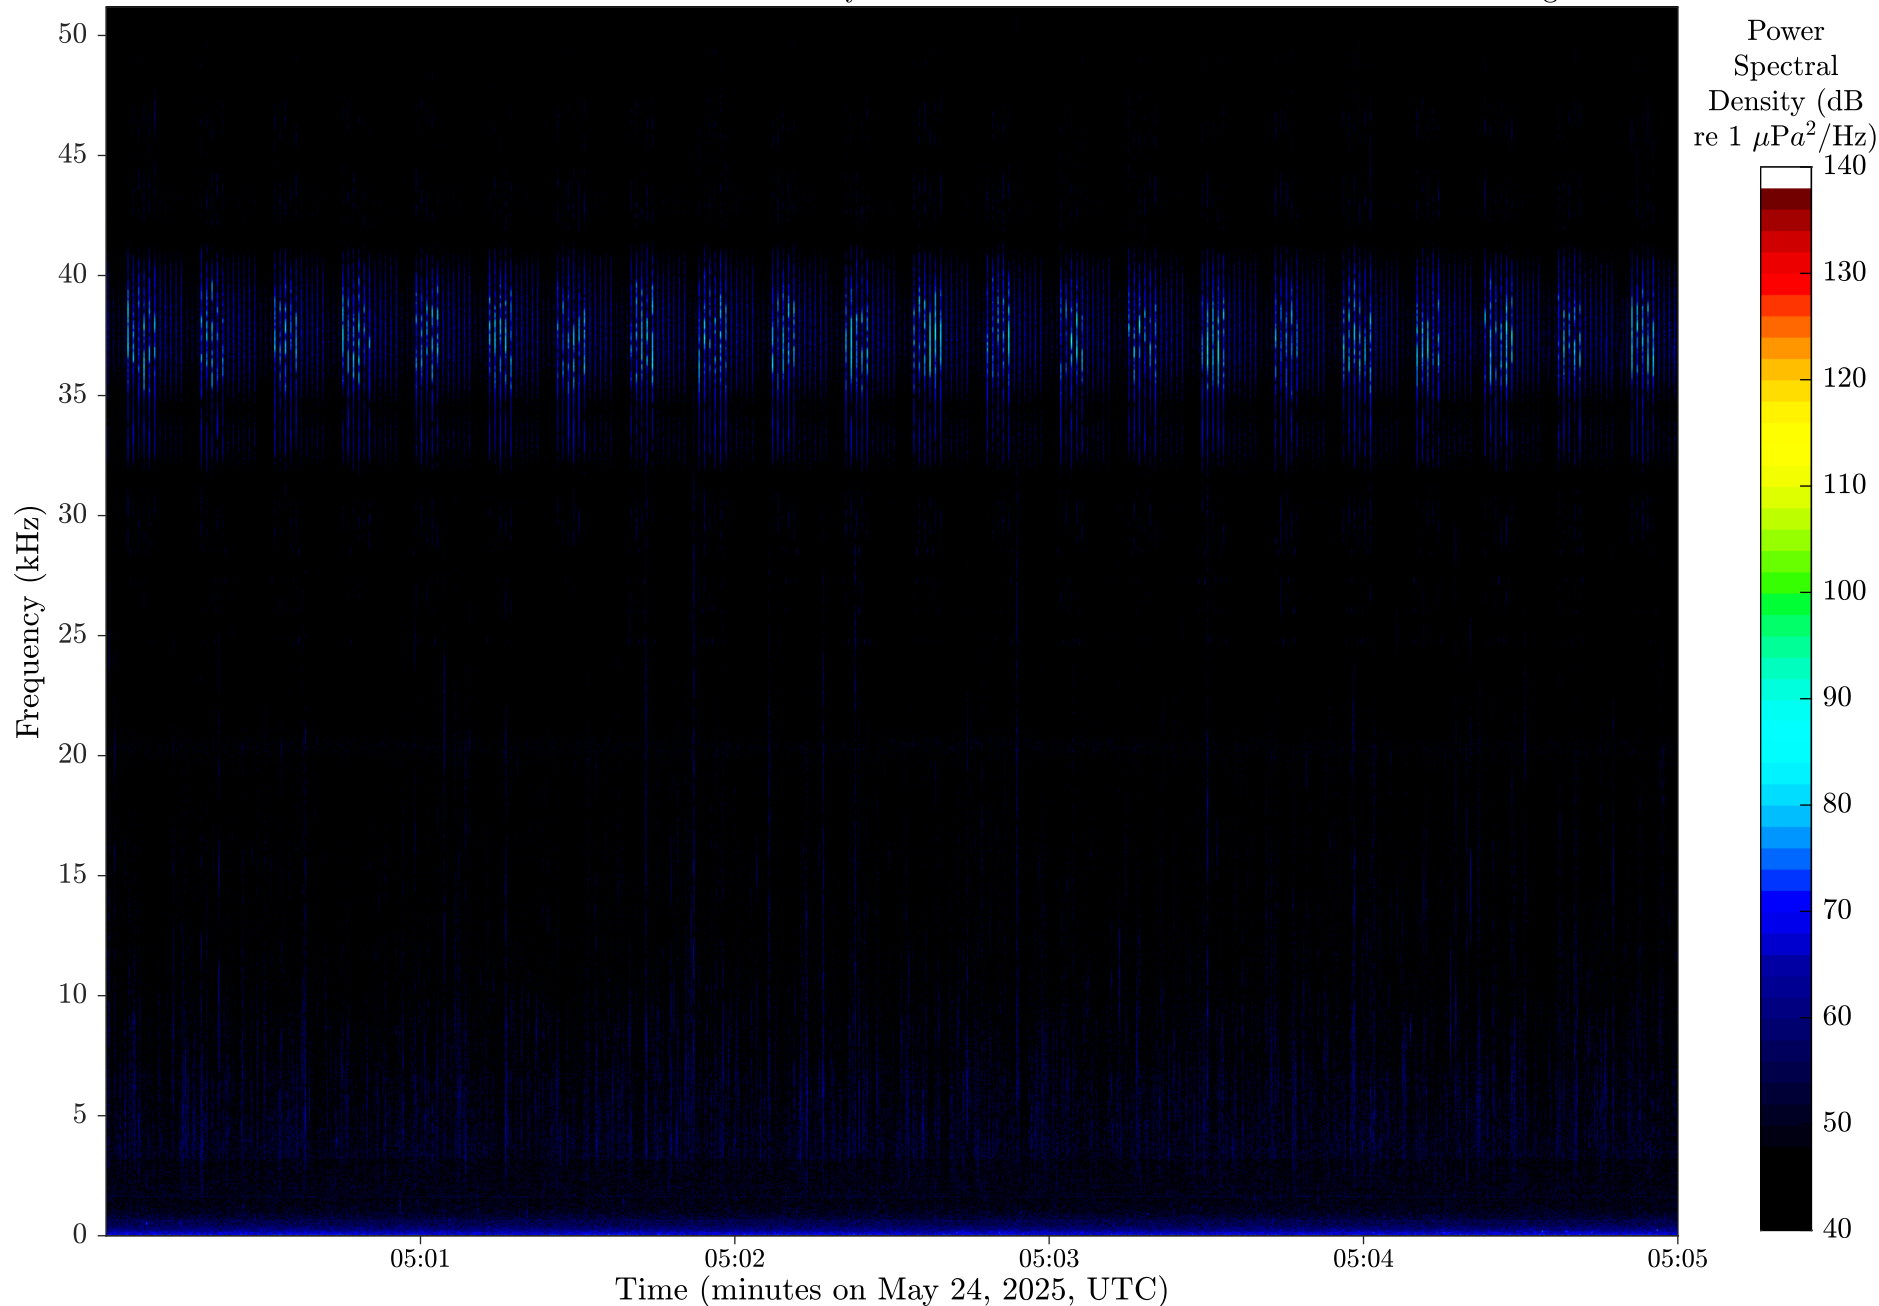


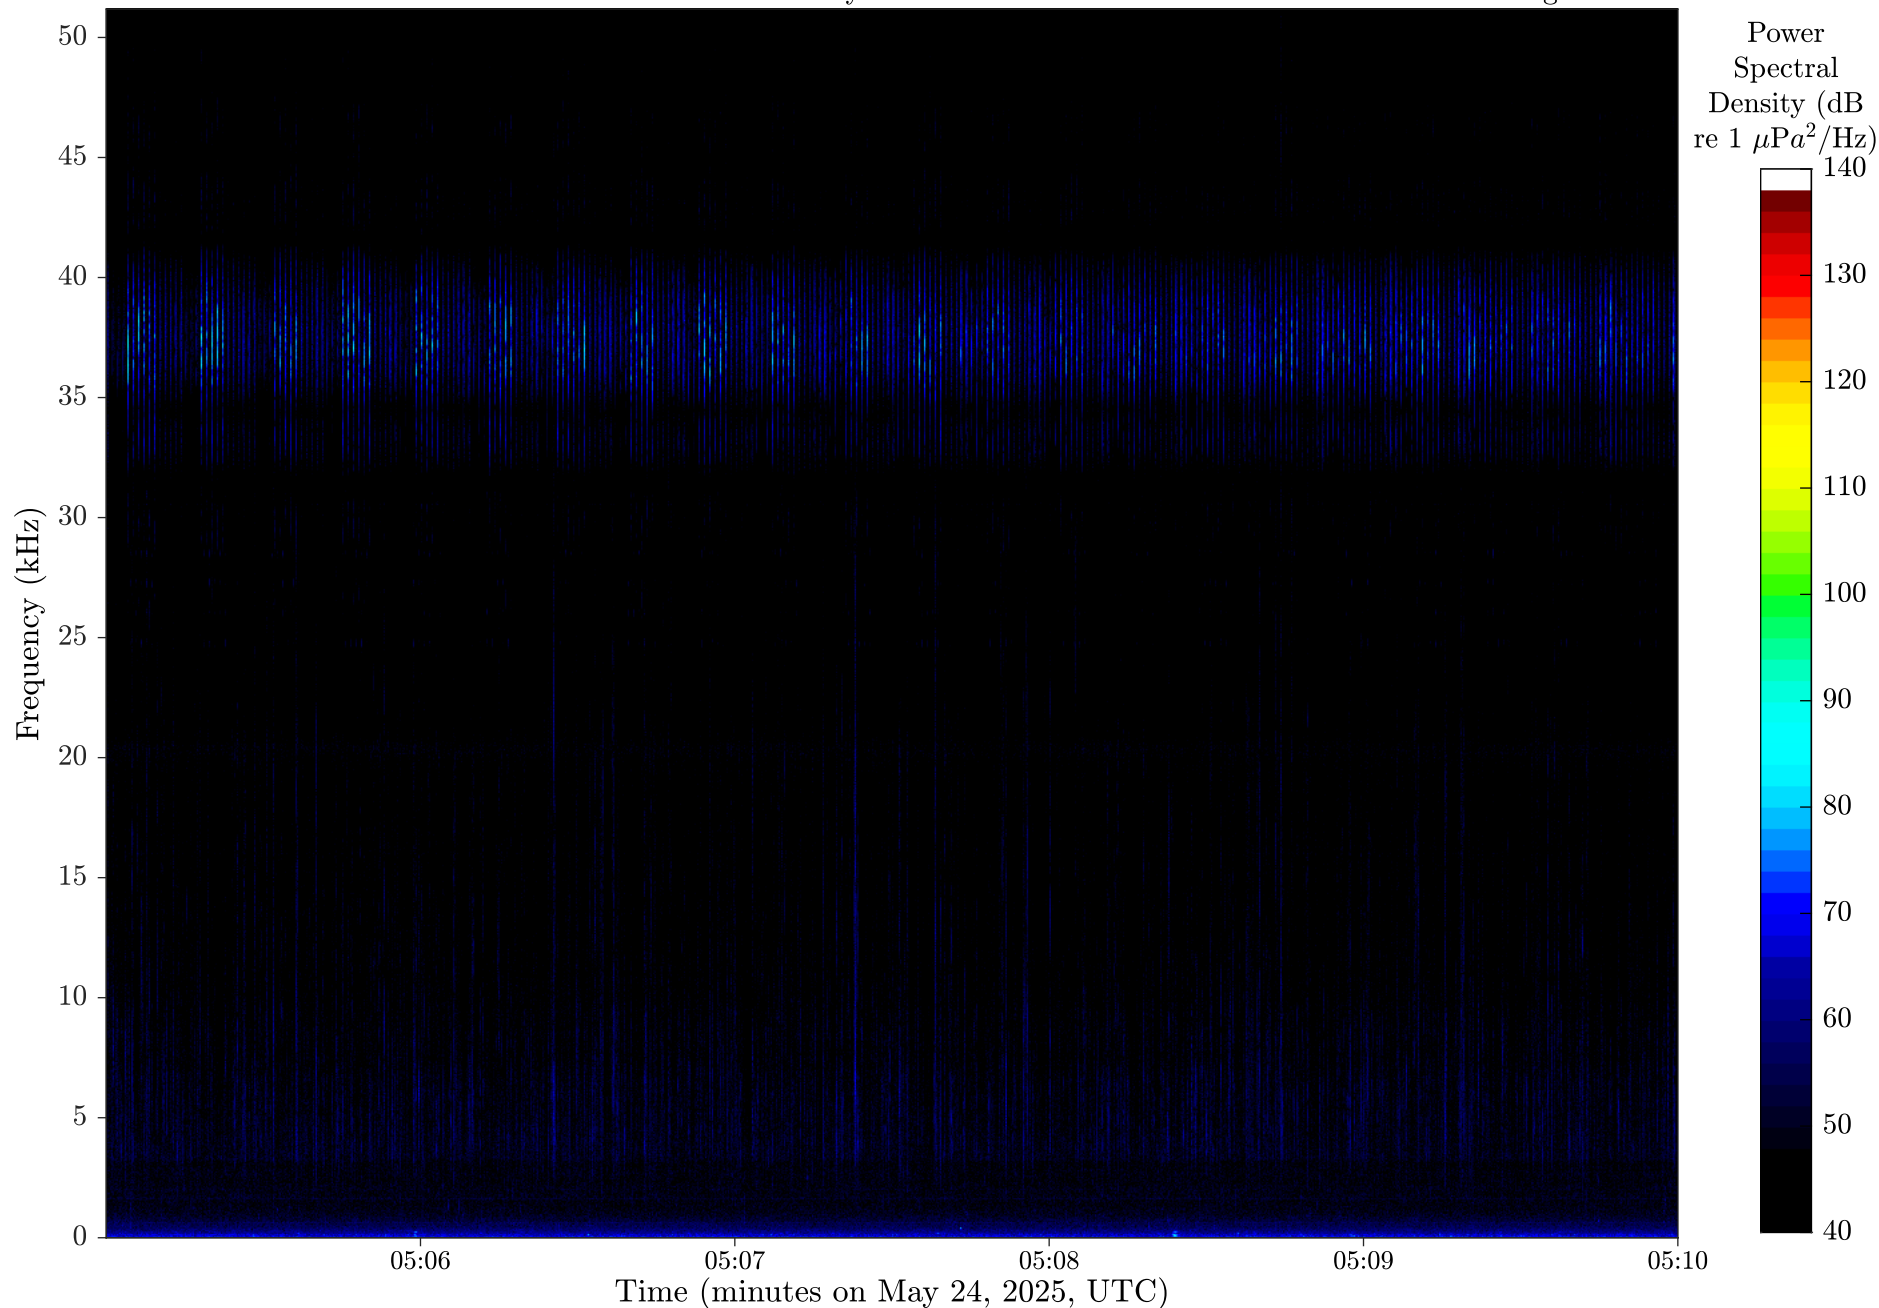


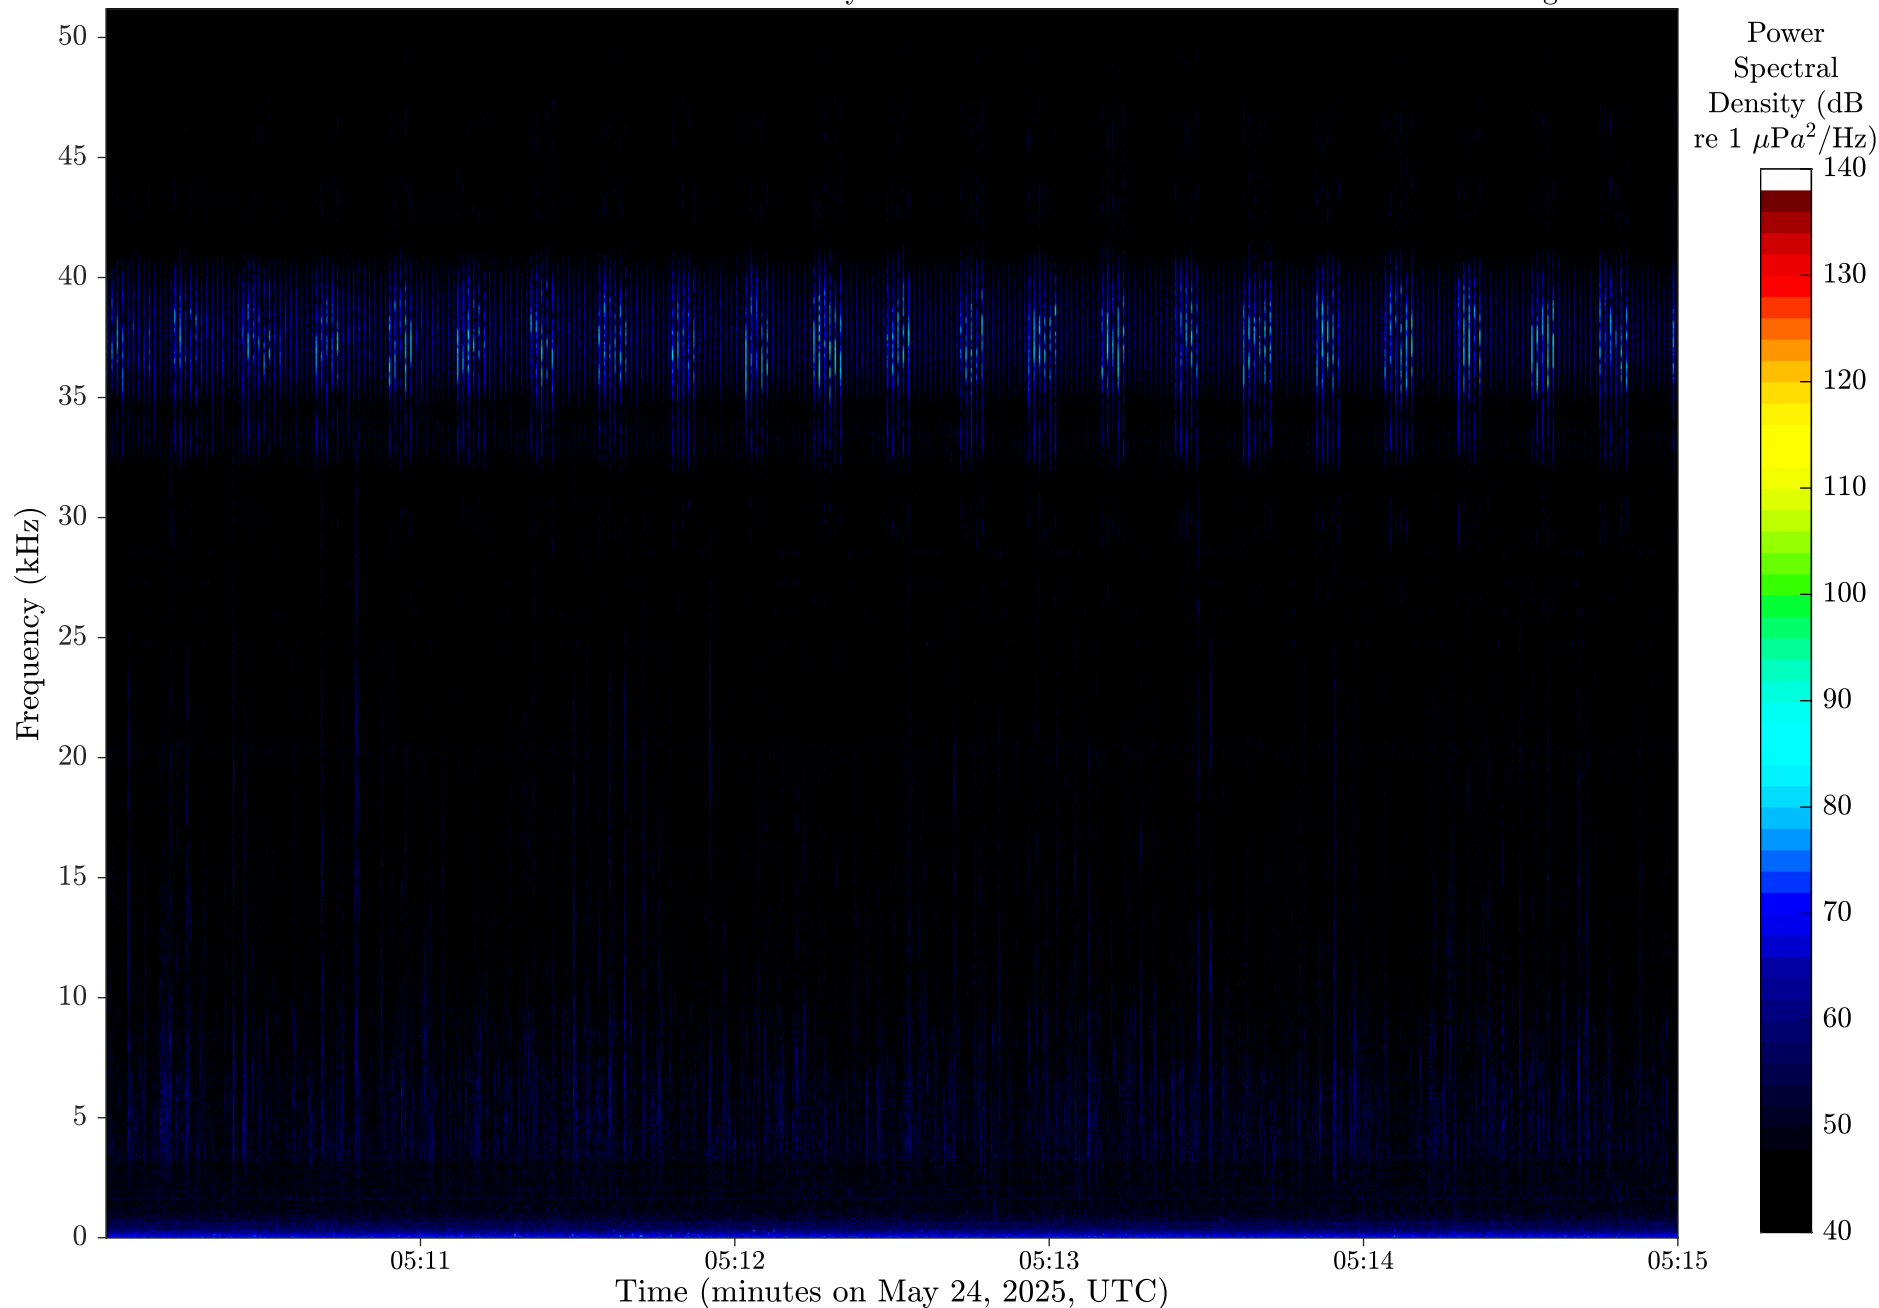

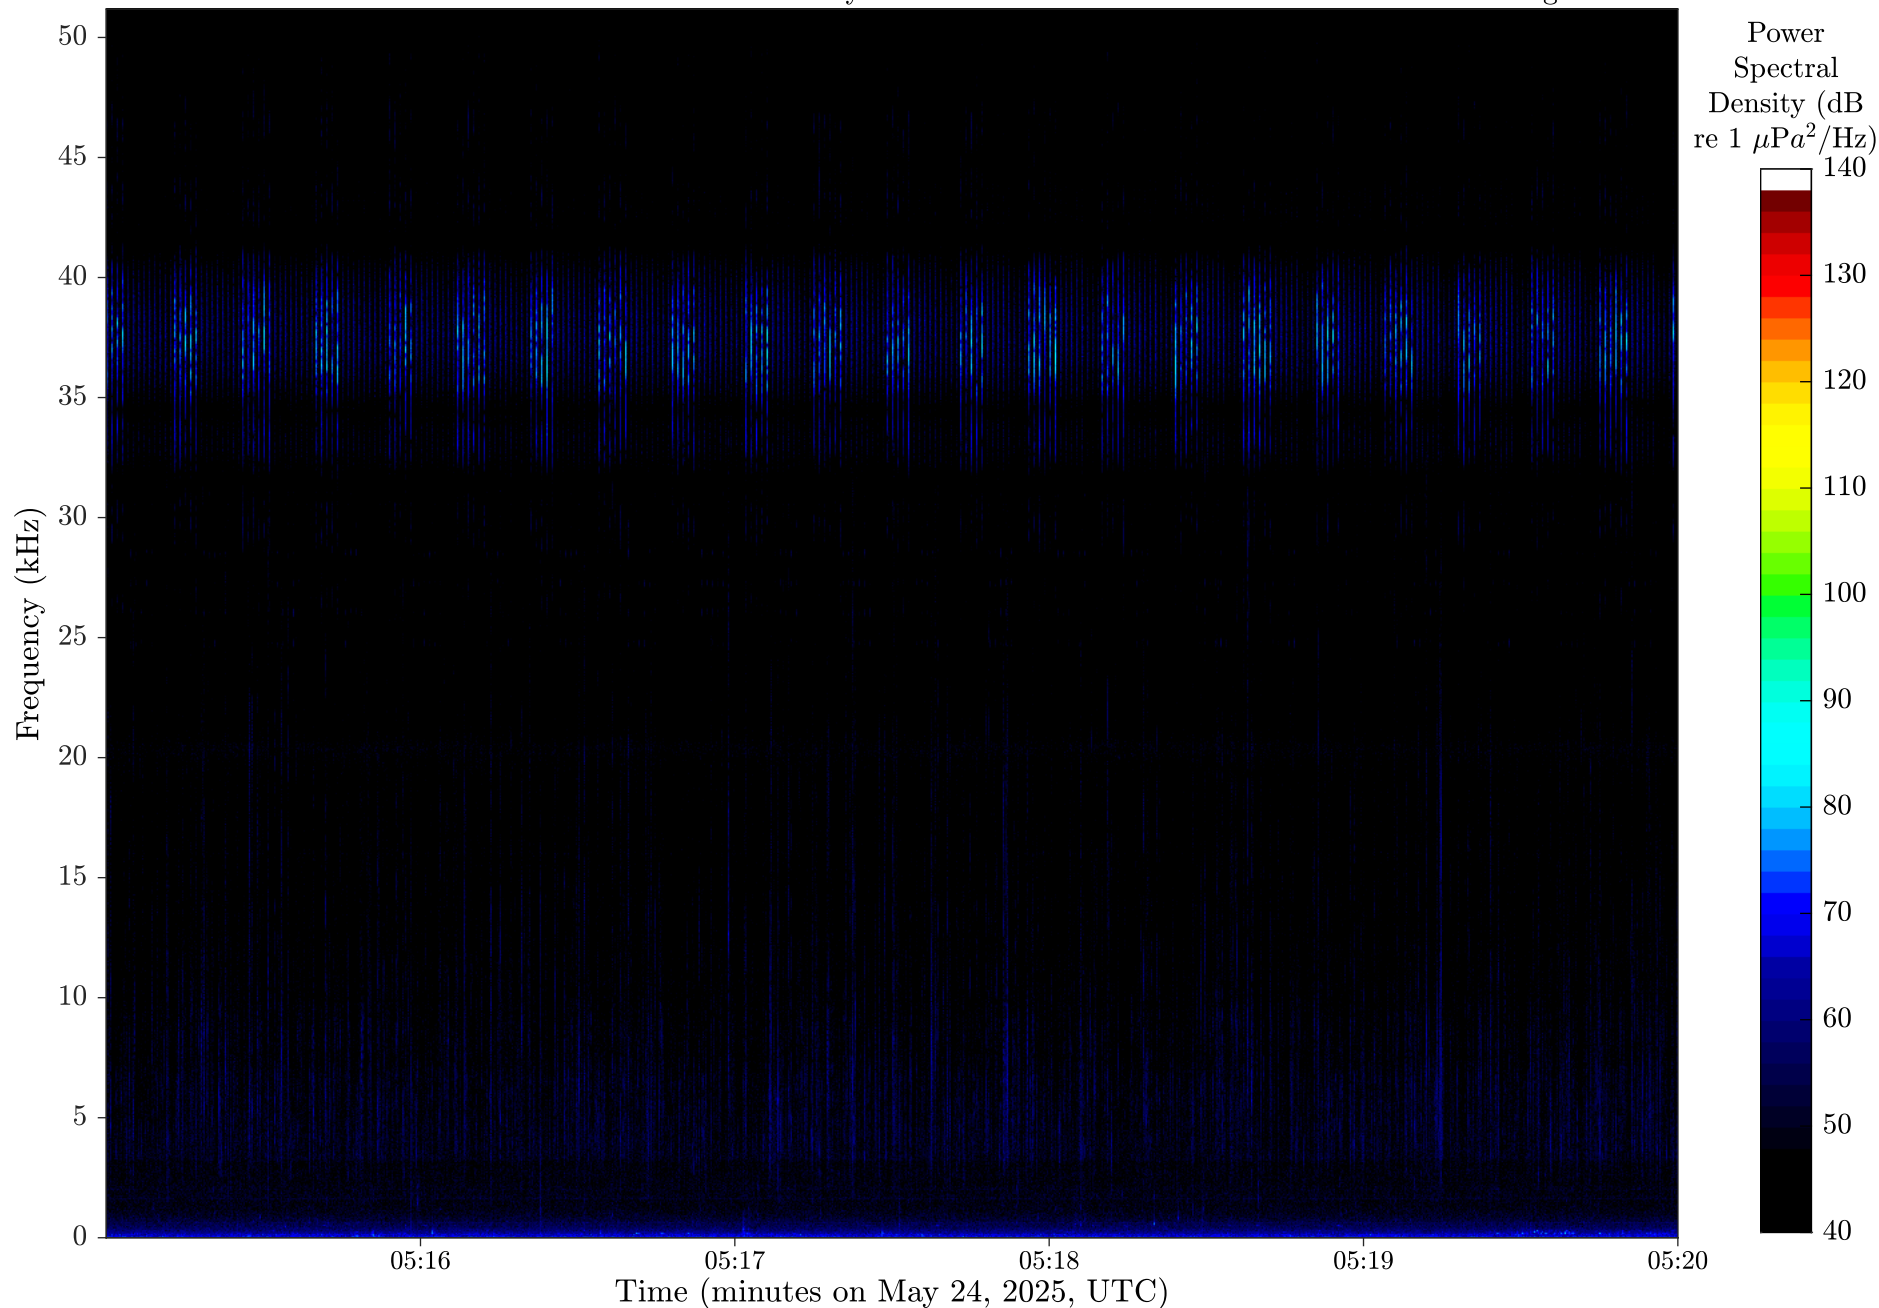

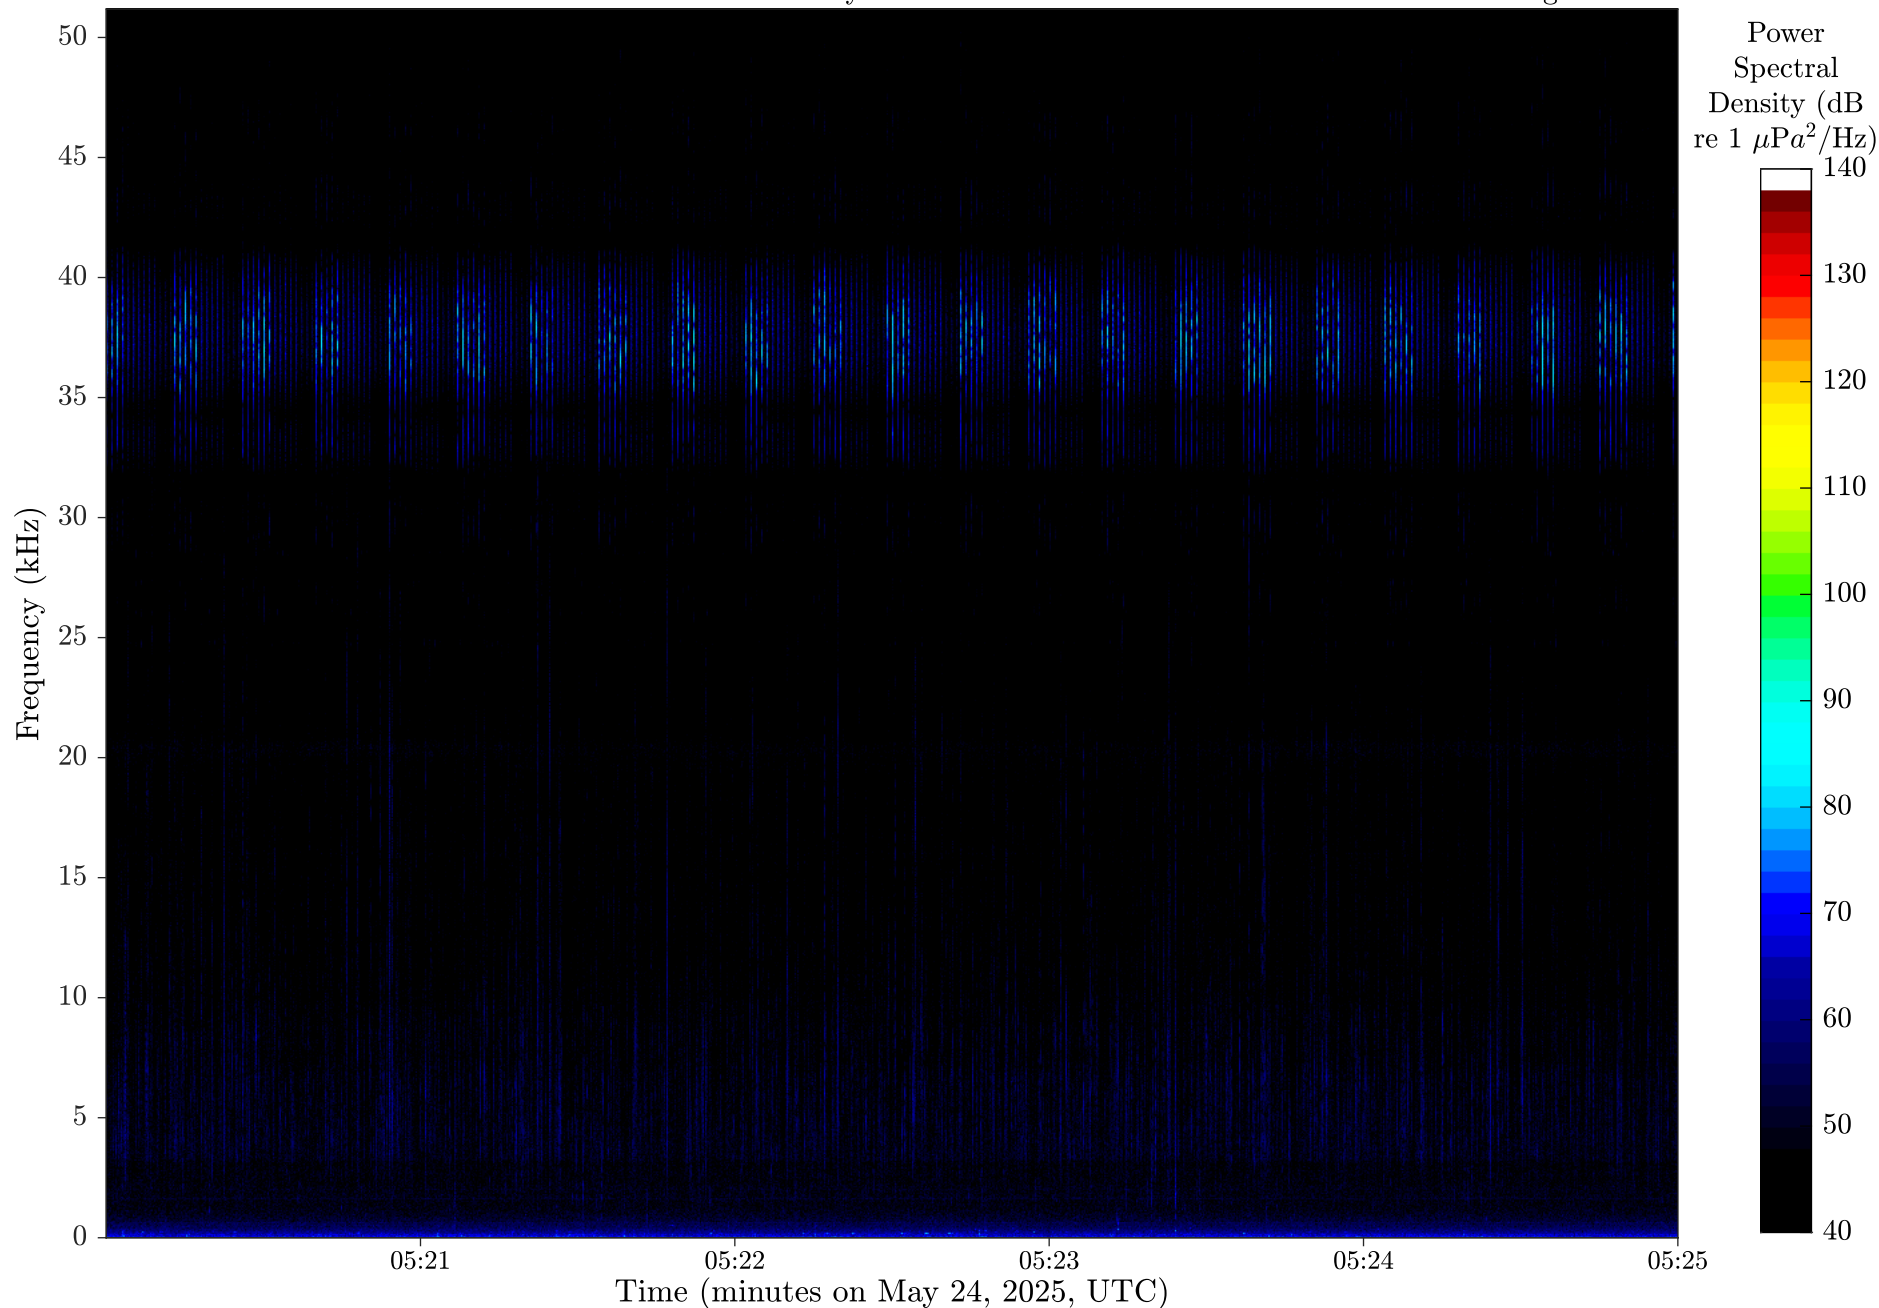


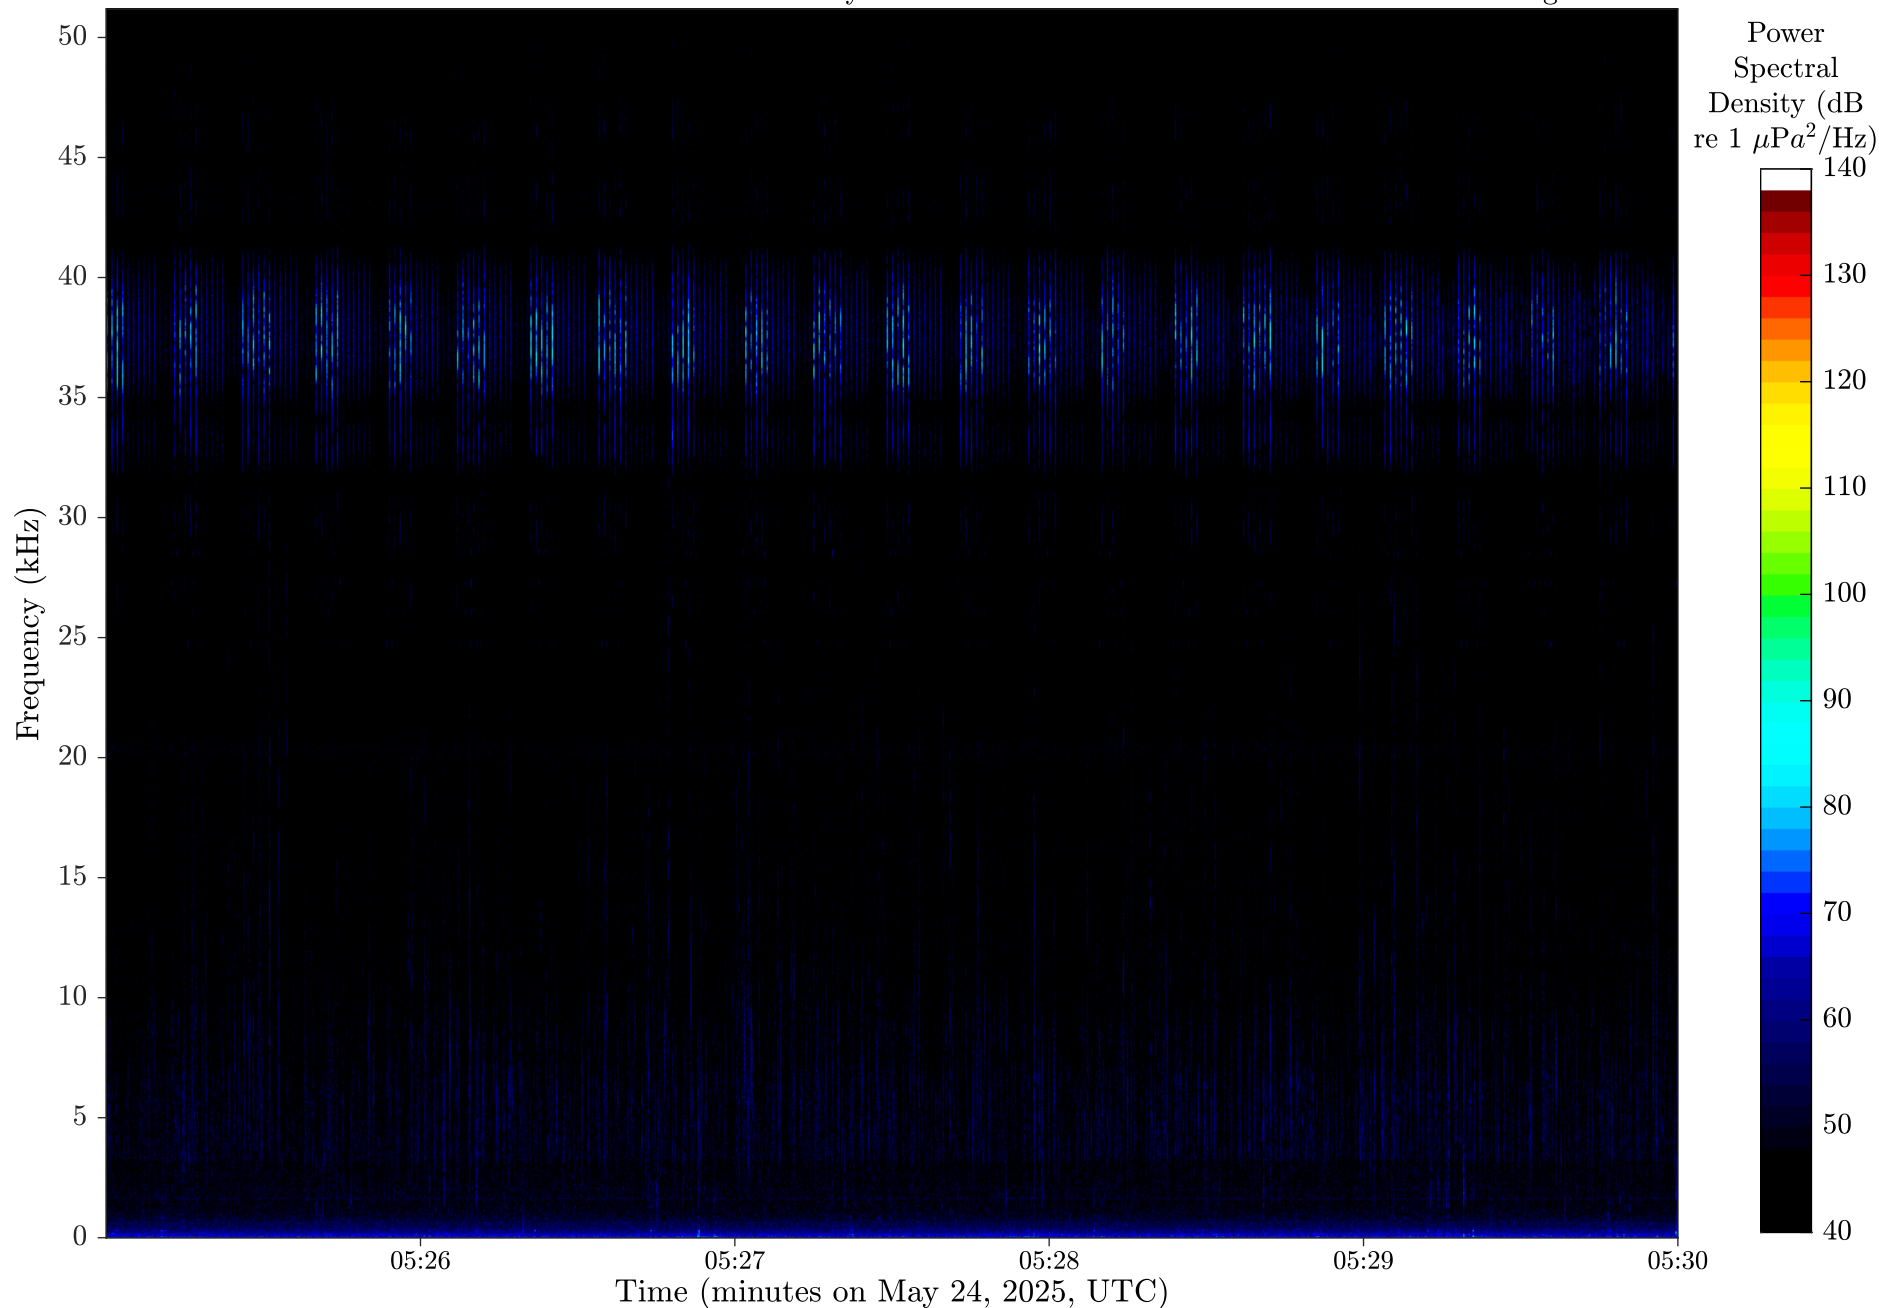

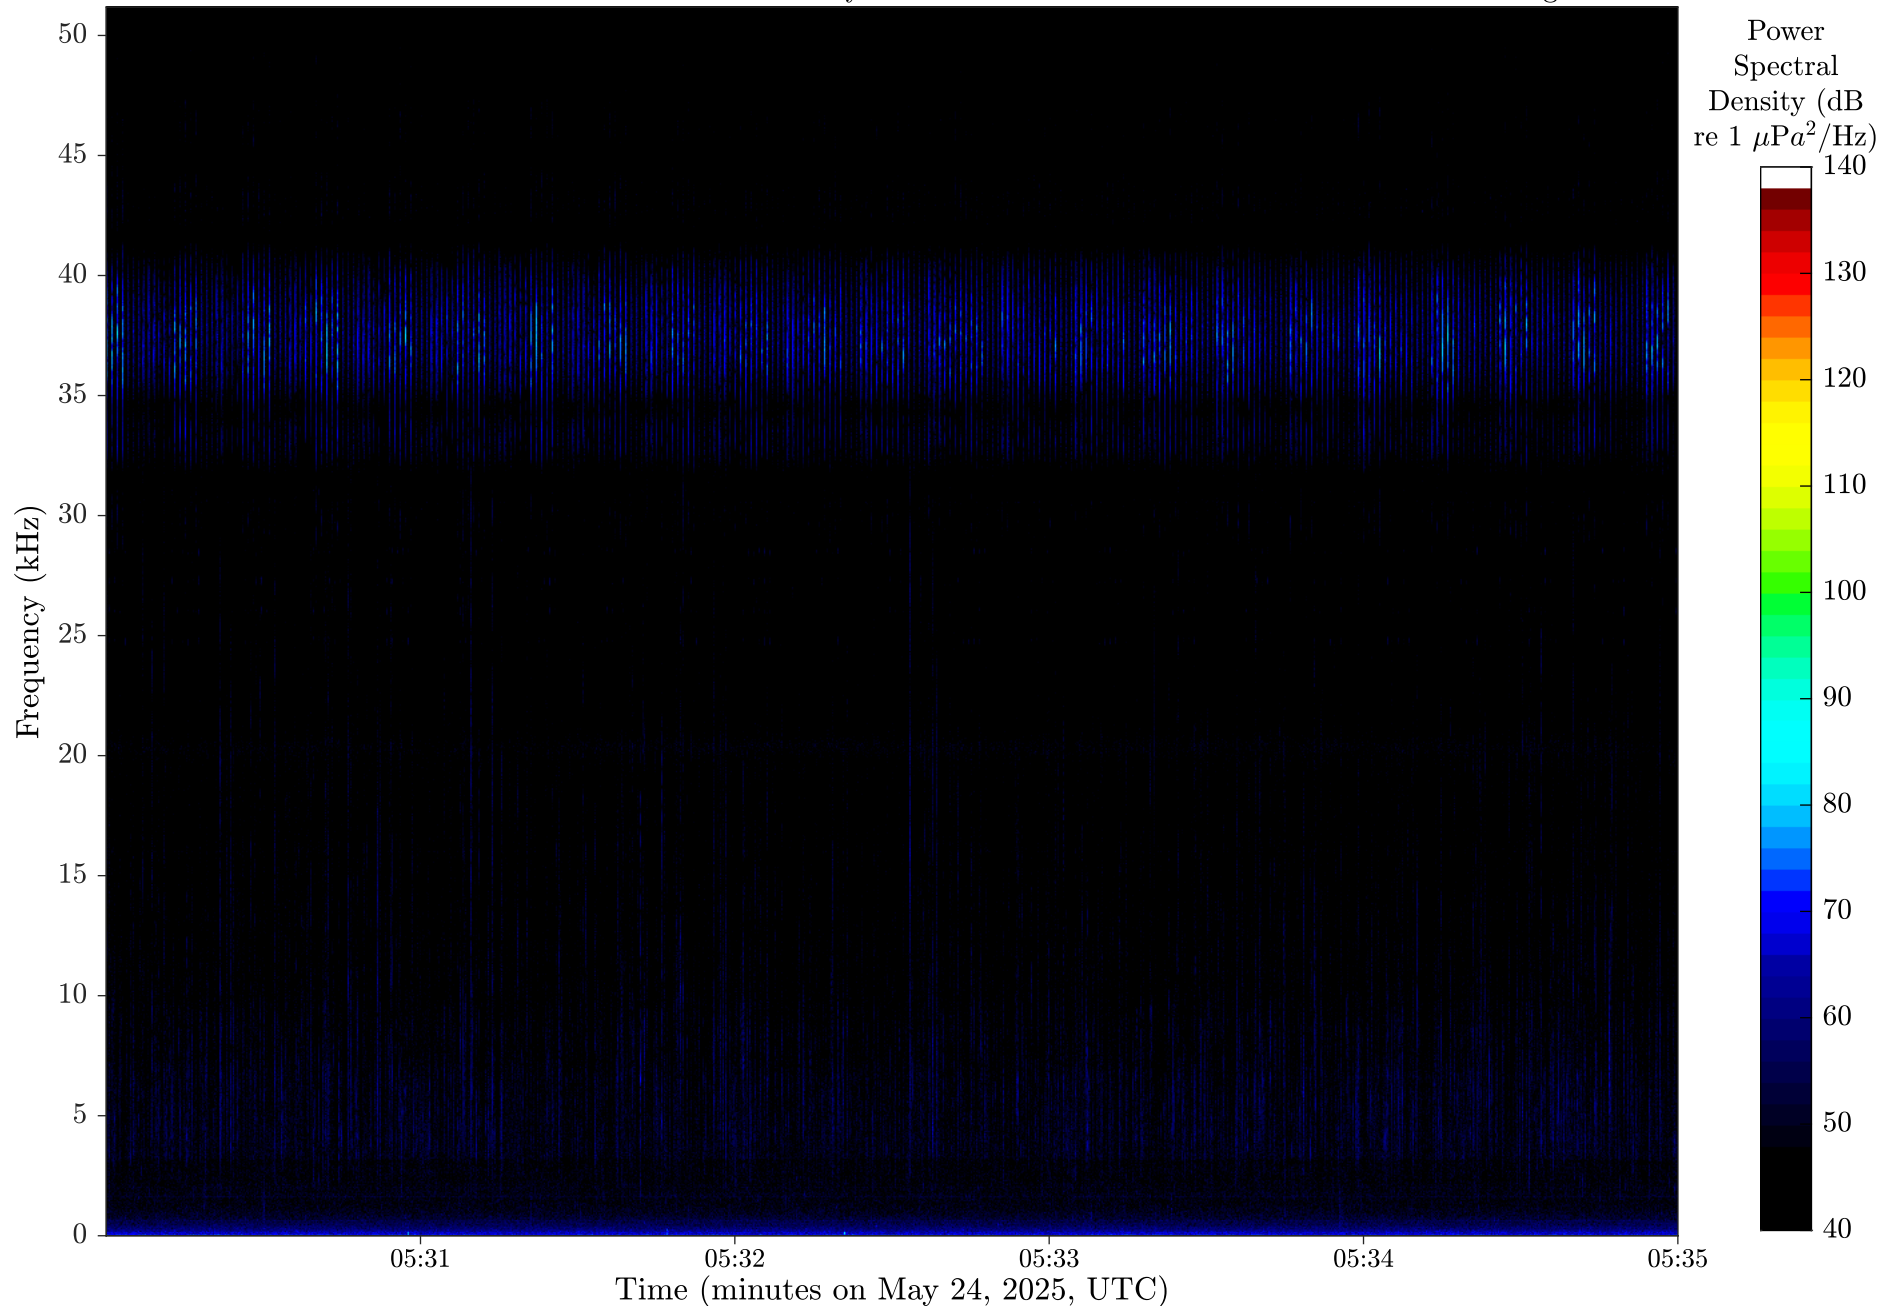


Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:16:29 UTC

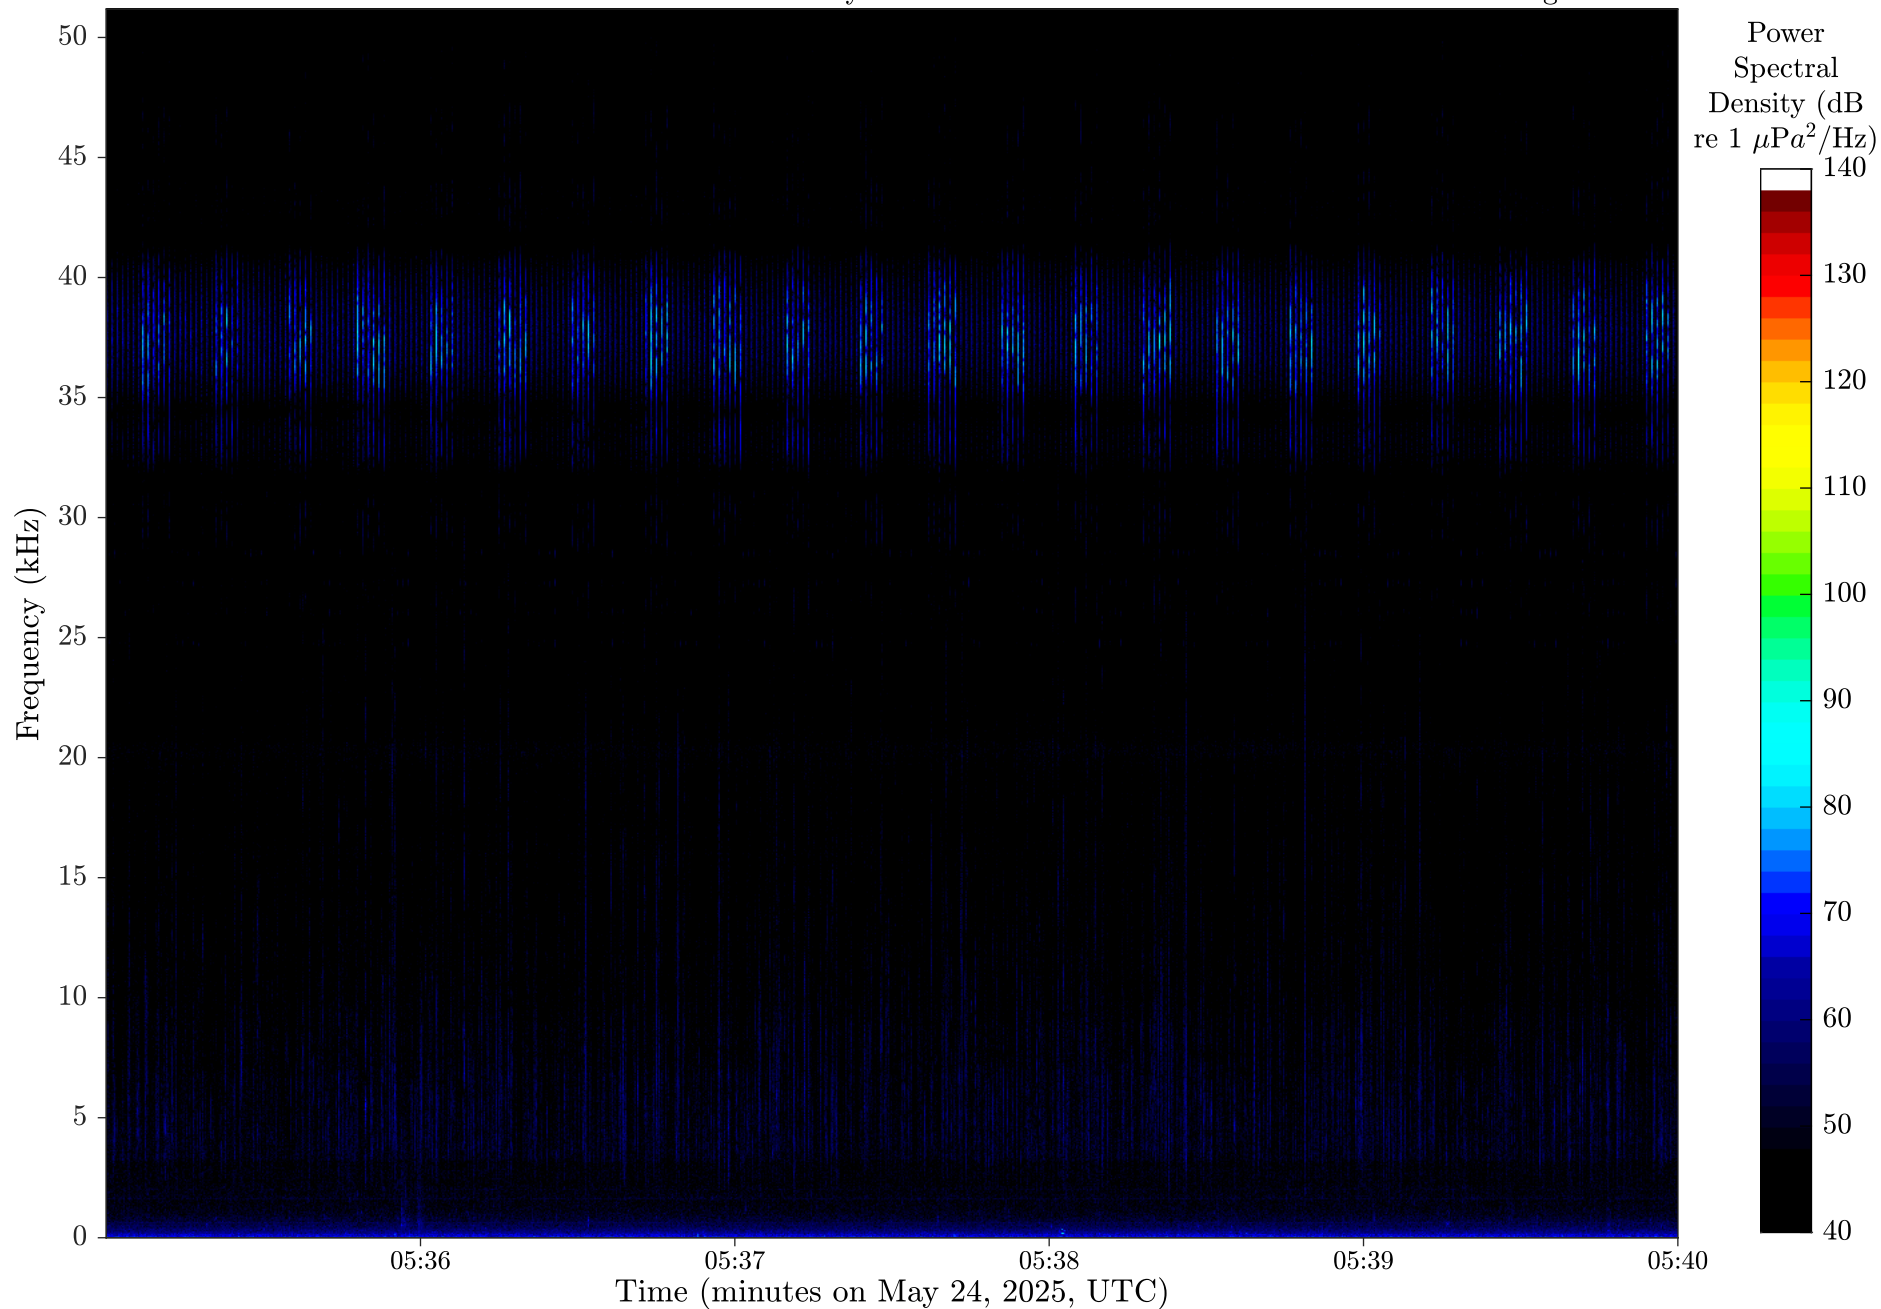


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:16:37 UTC

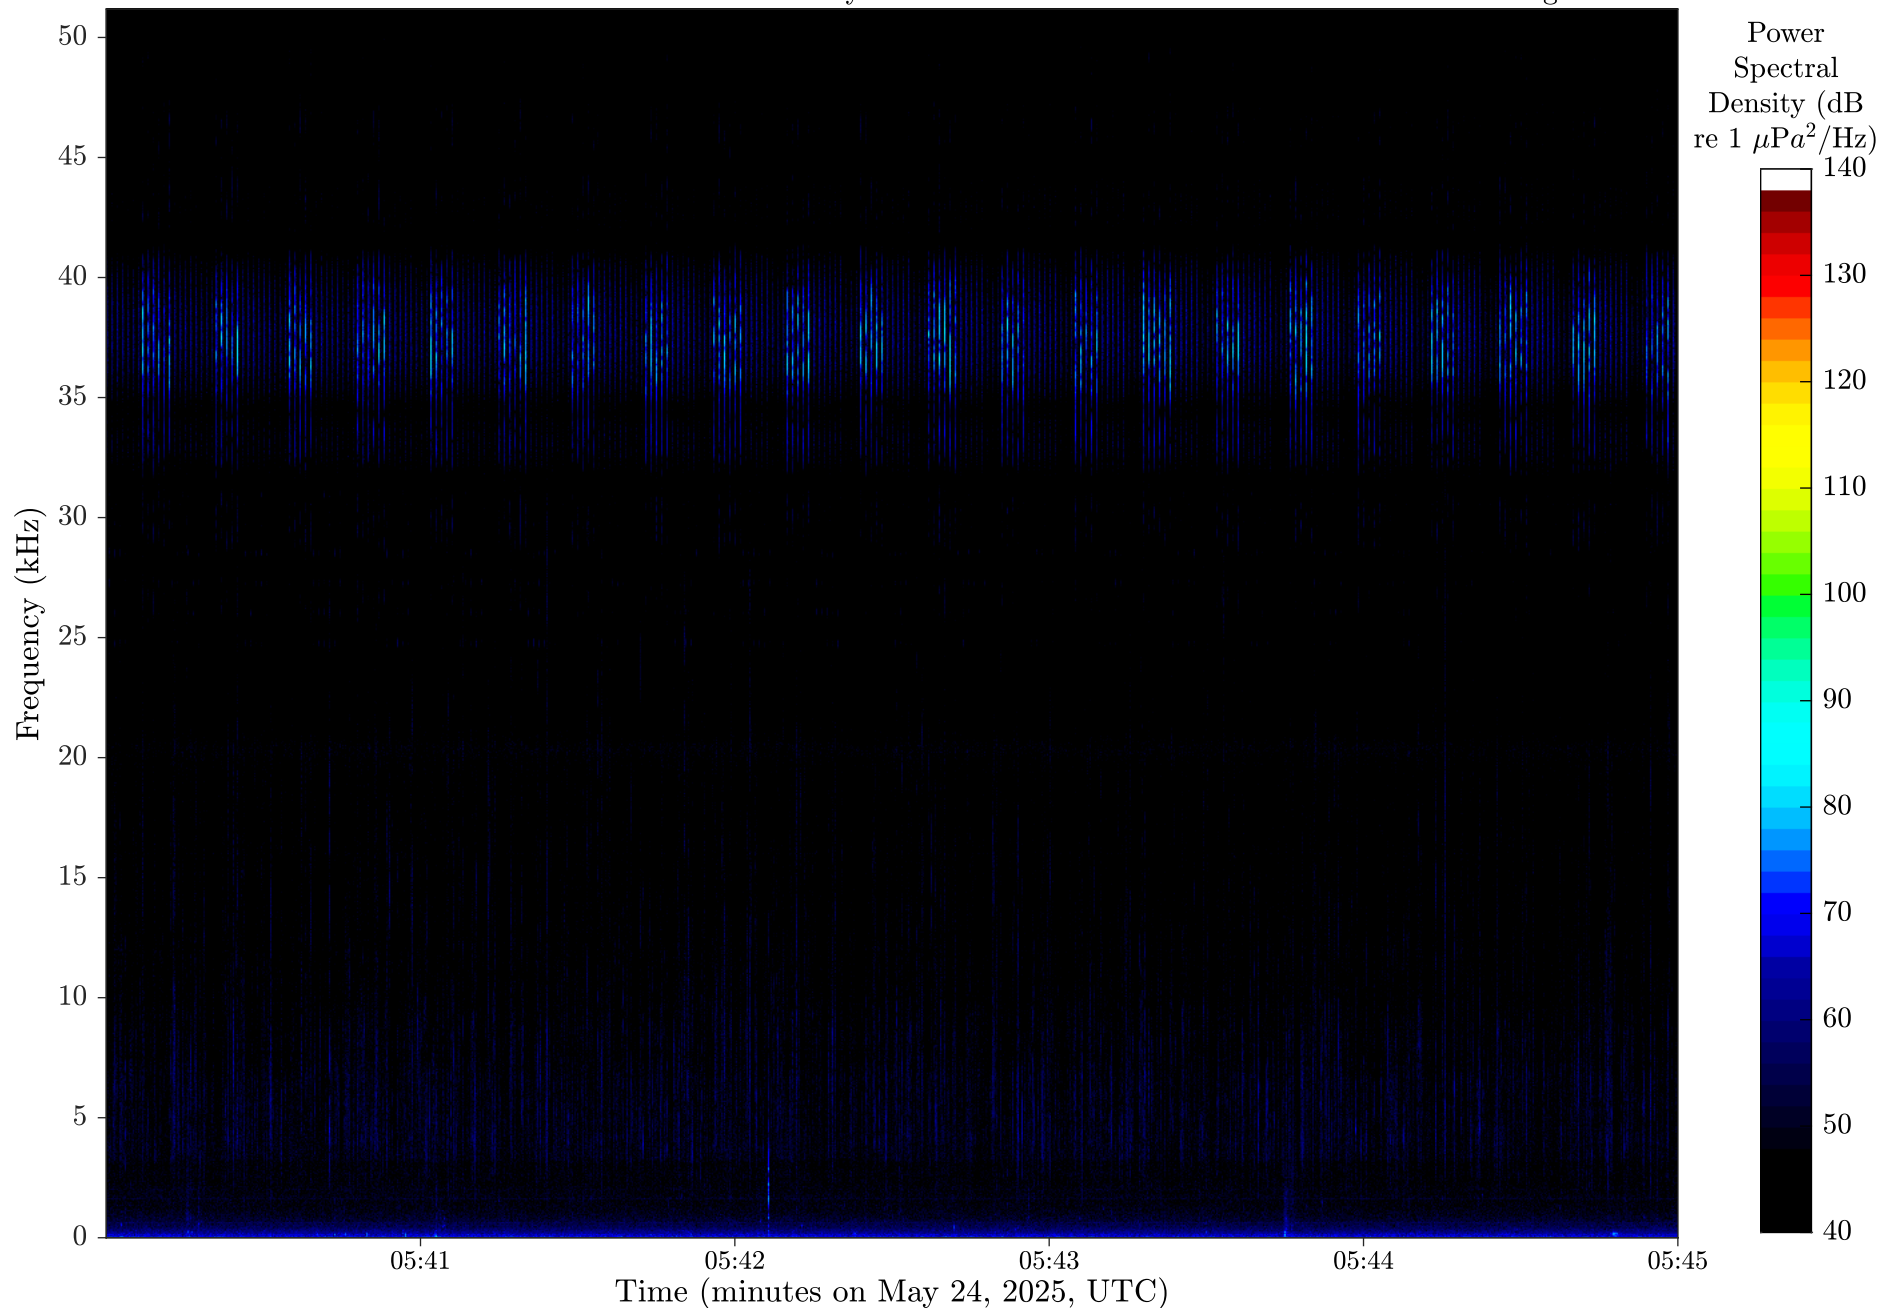


Comments: 36.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:16:45 UTC

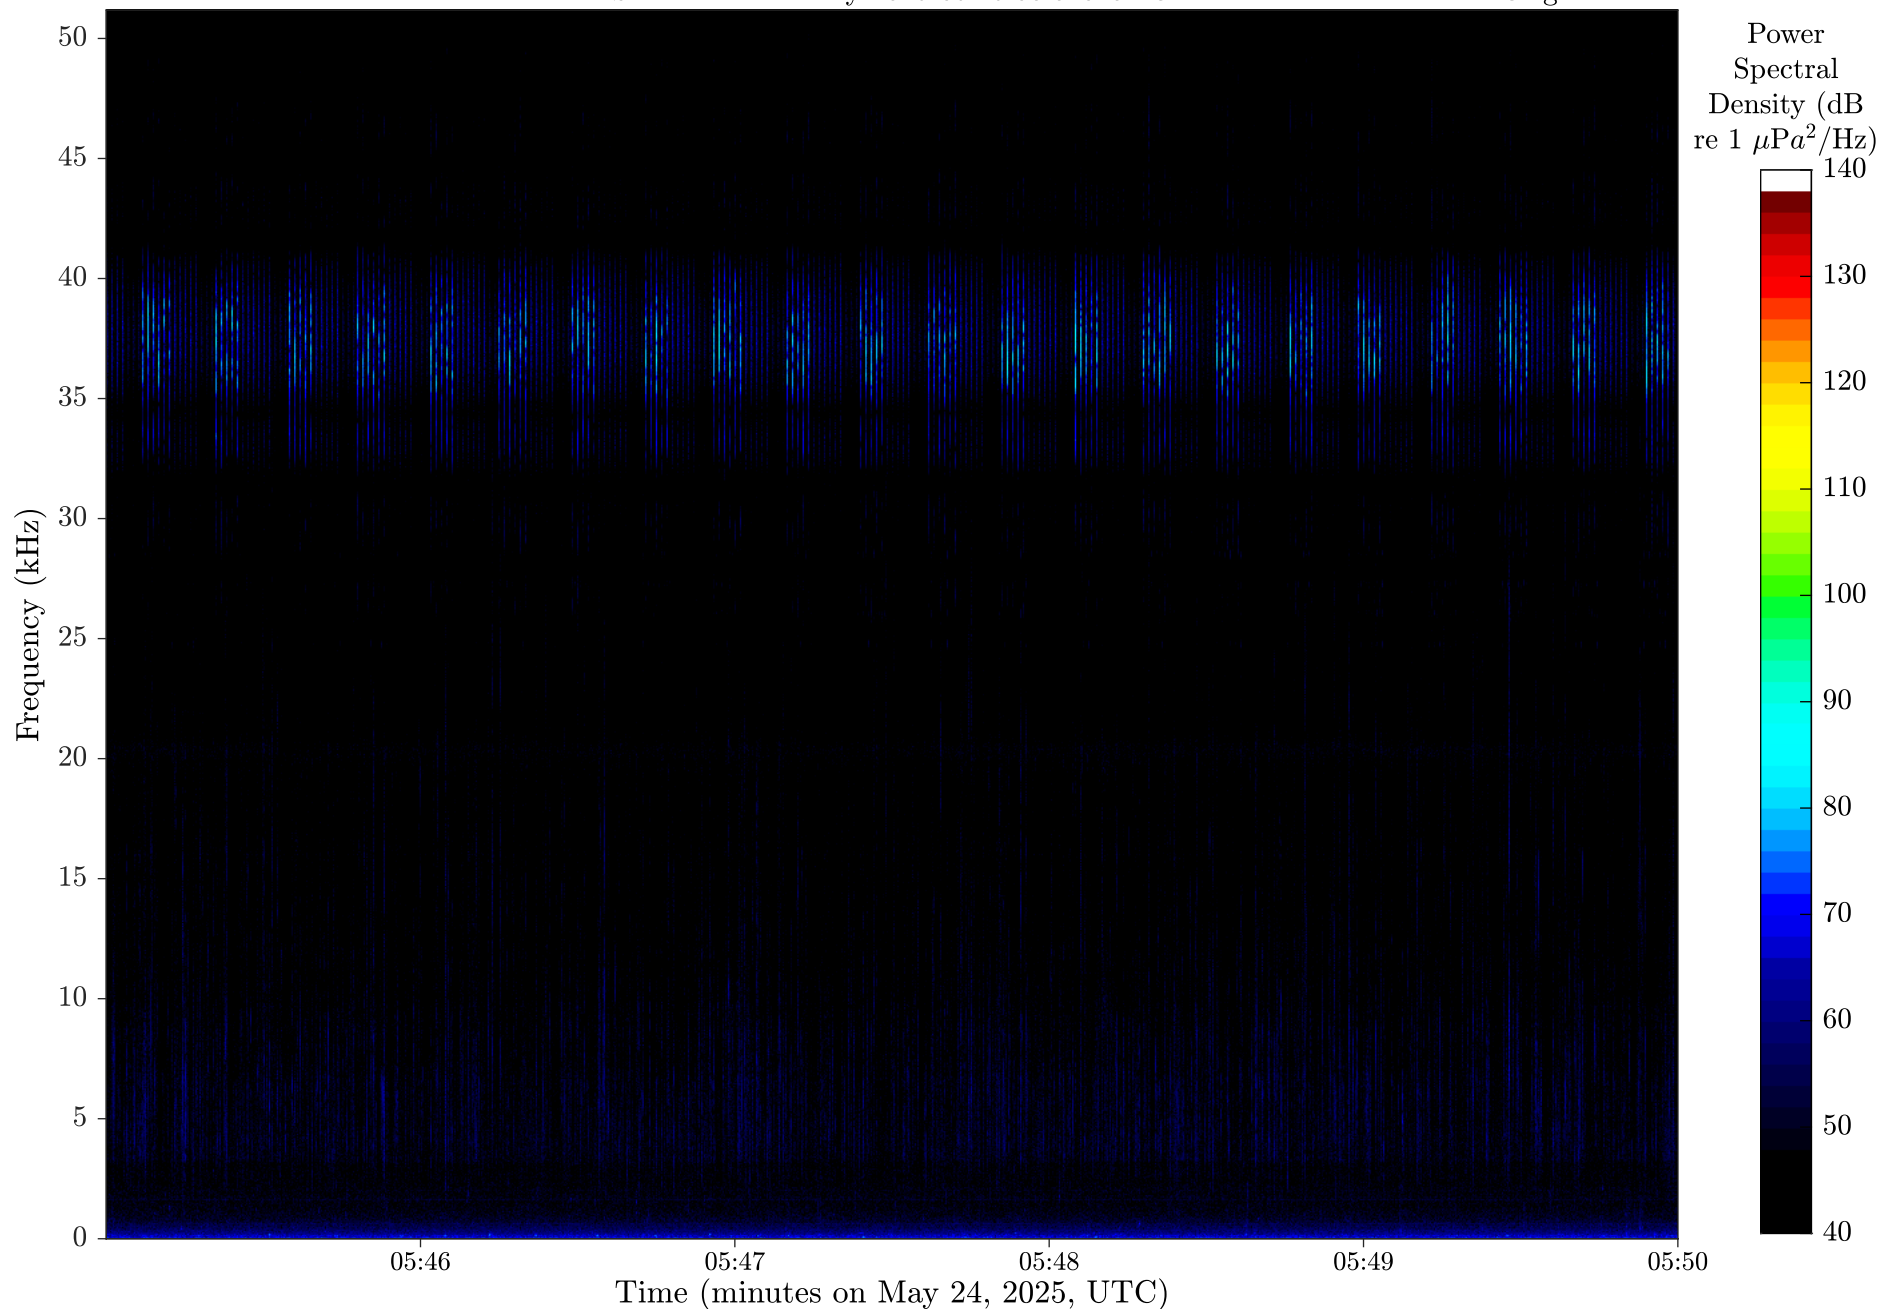


Comments: 36.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:16:54 UTC

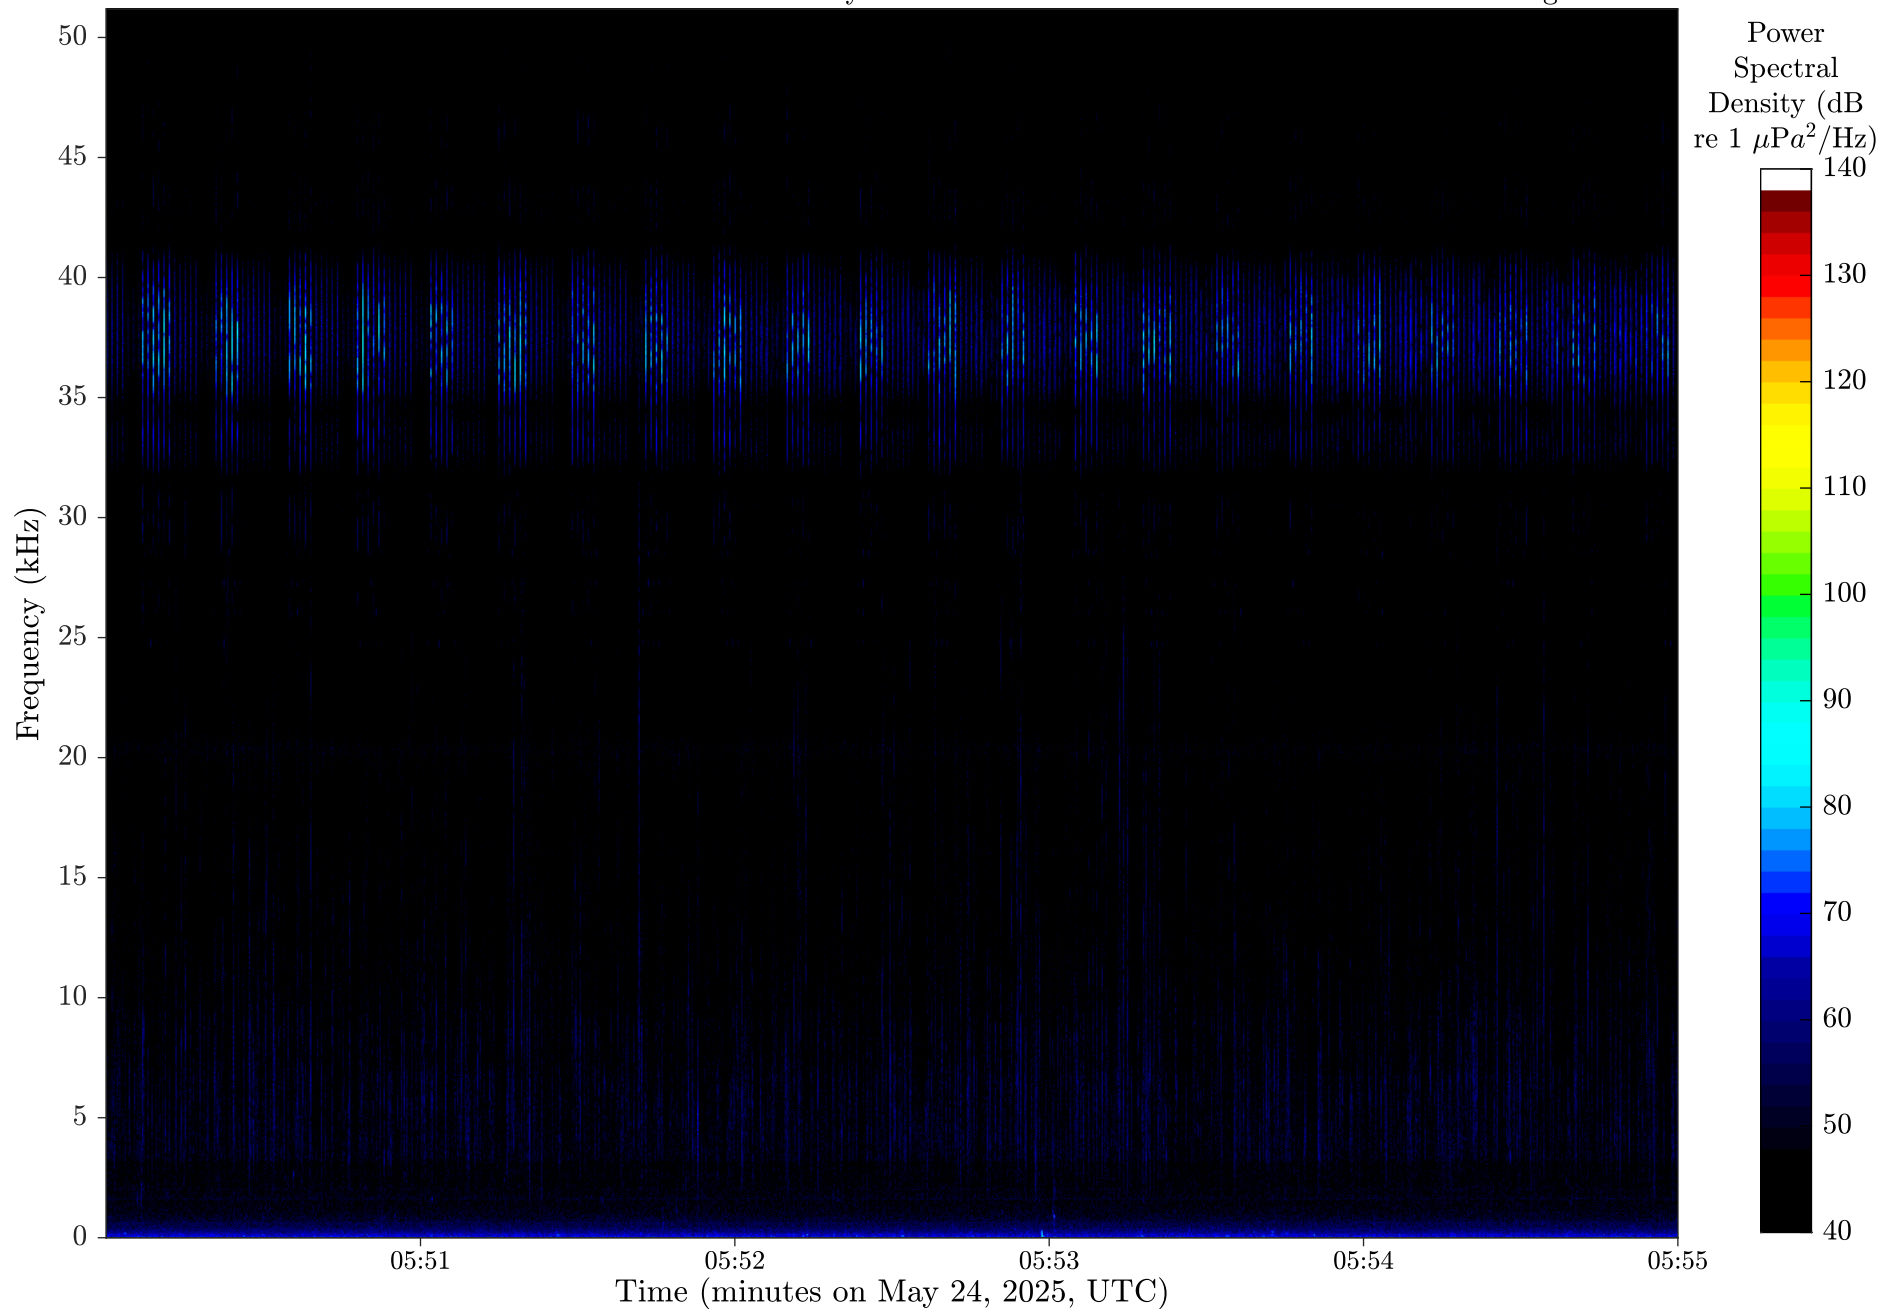

Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:17:02 UTC

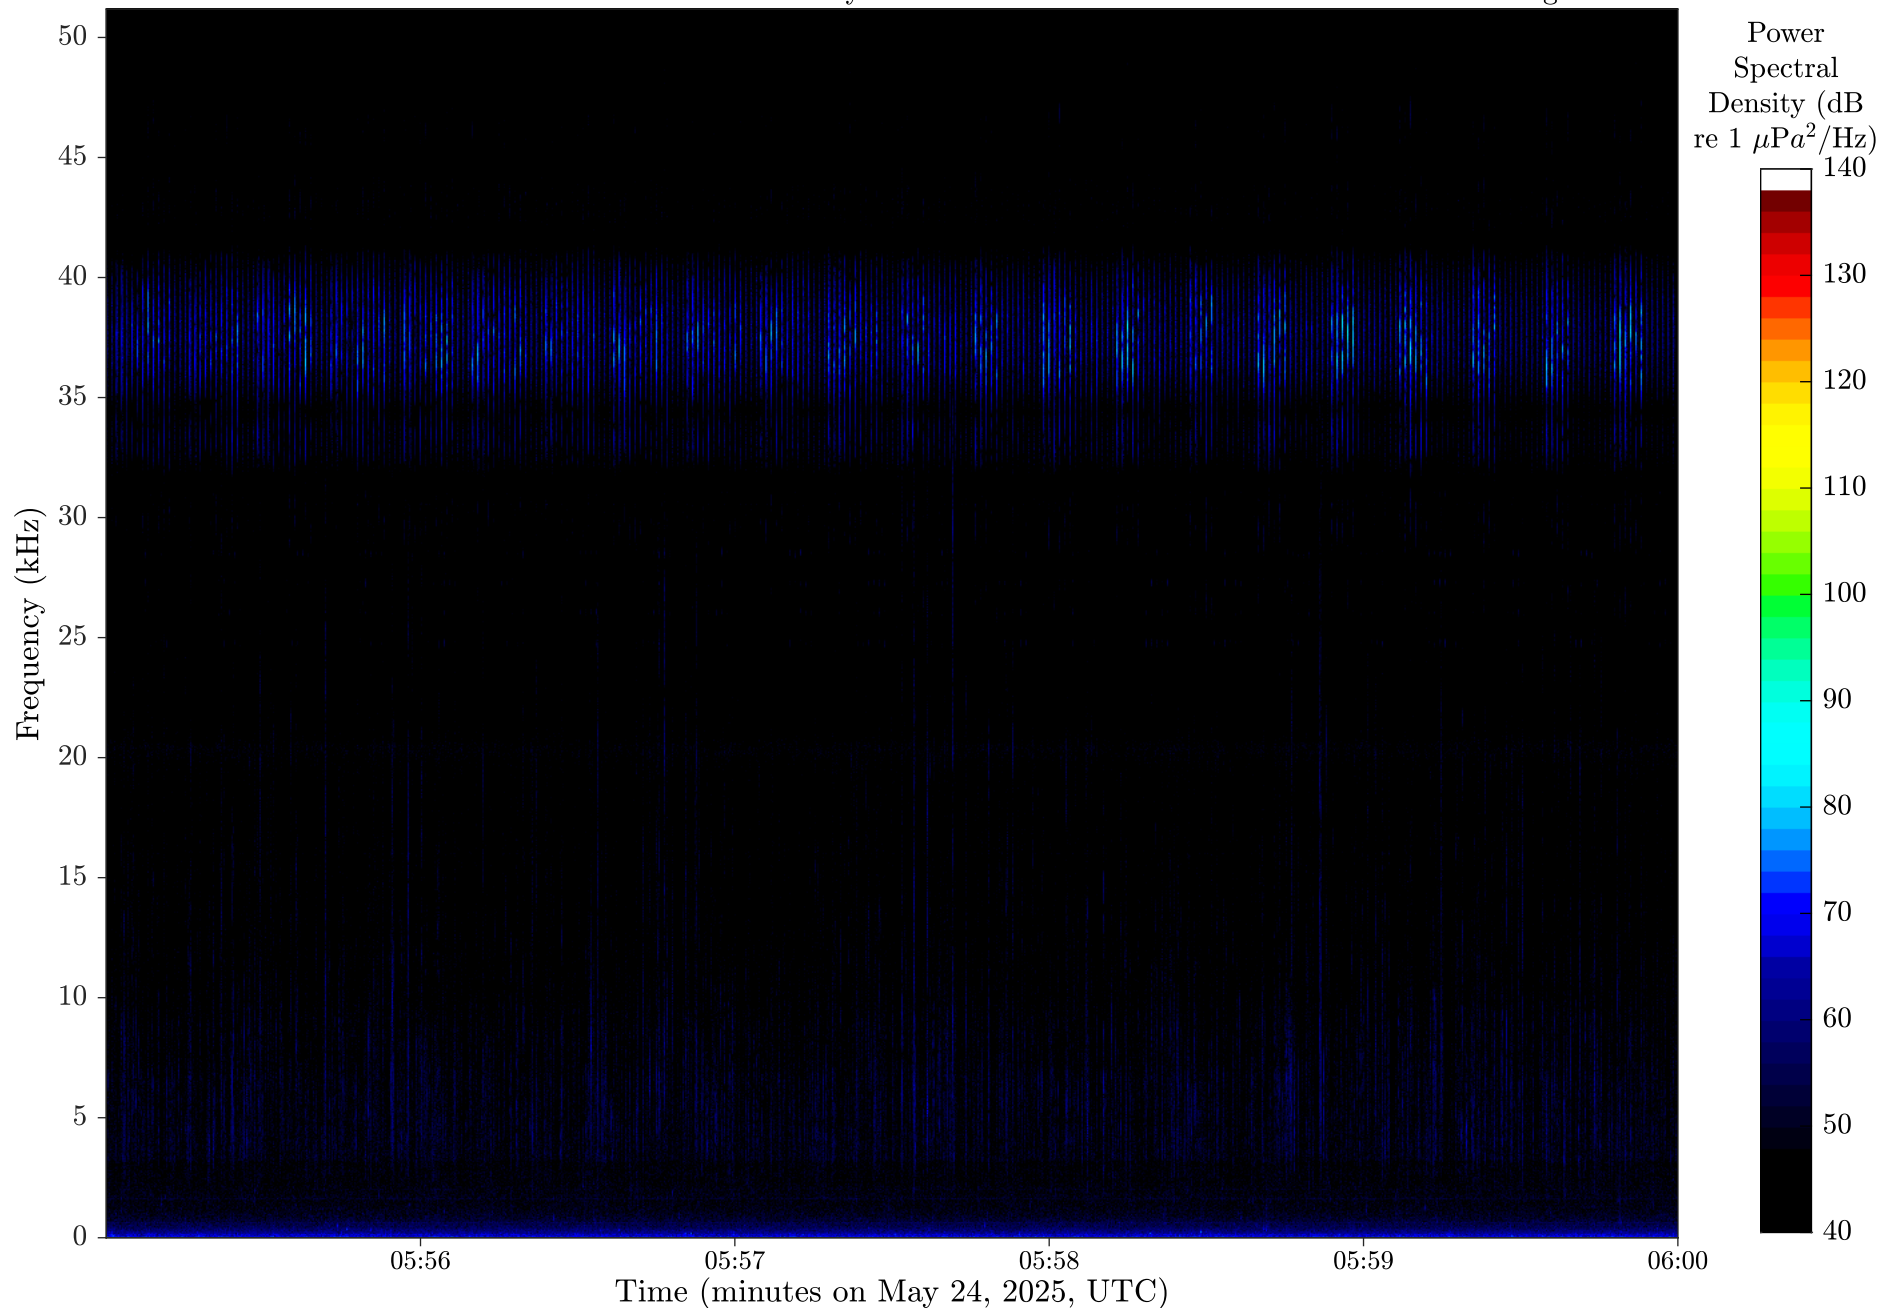

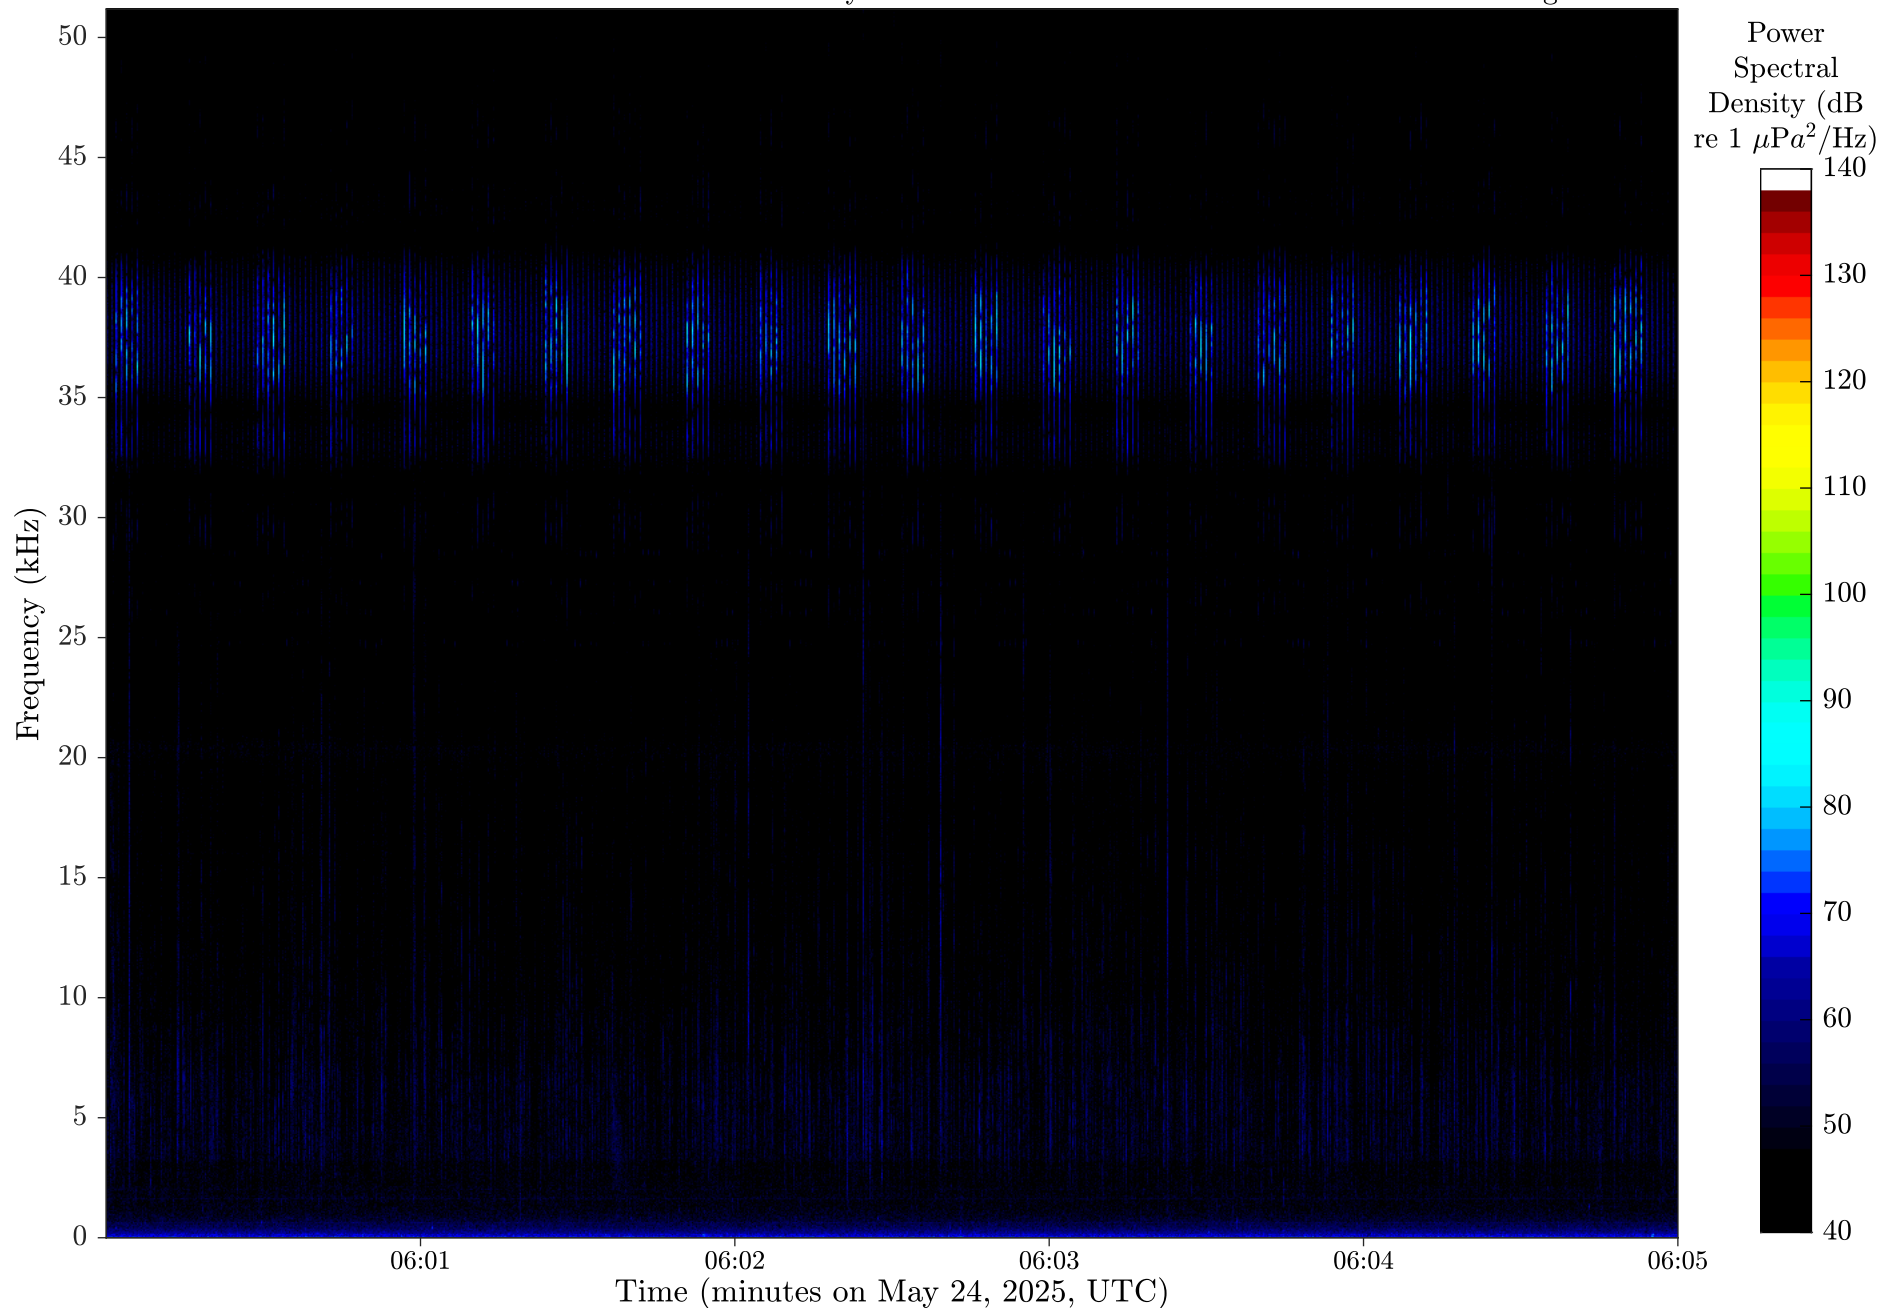


Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:17:18 UTC

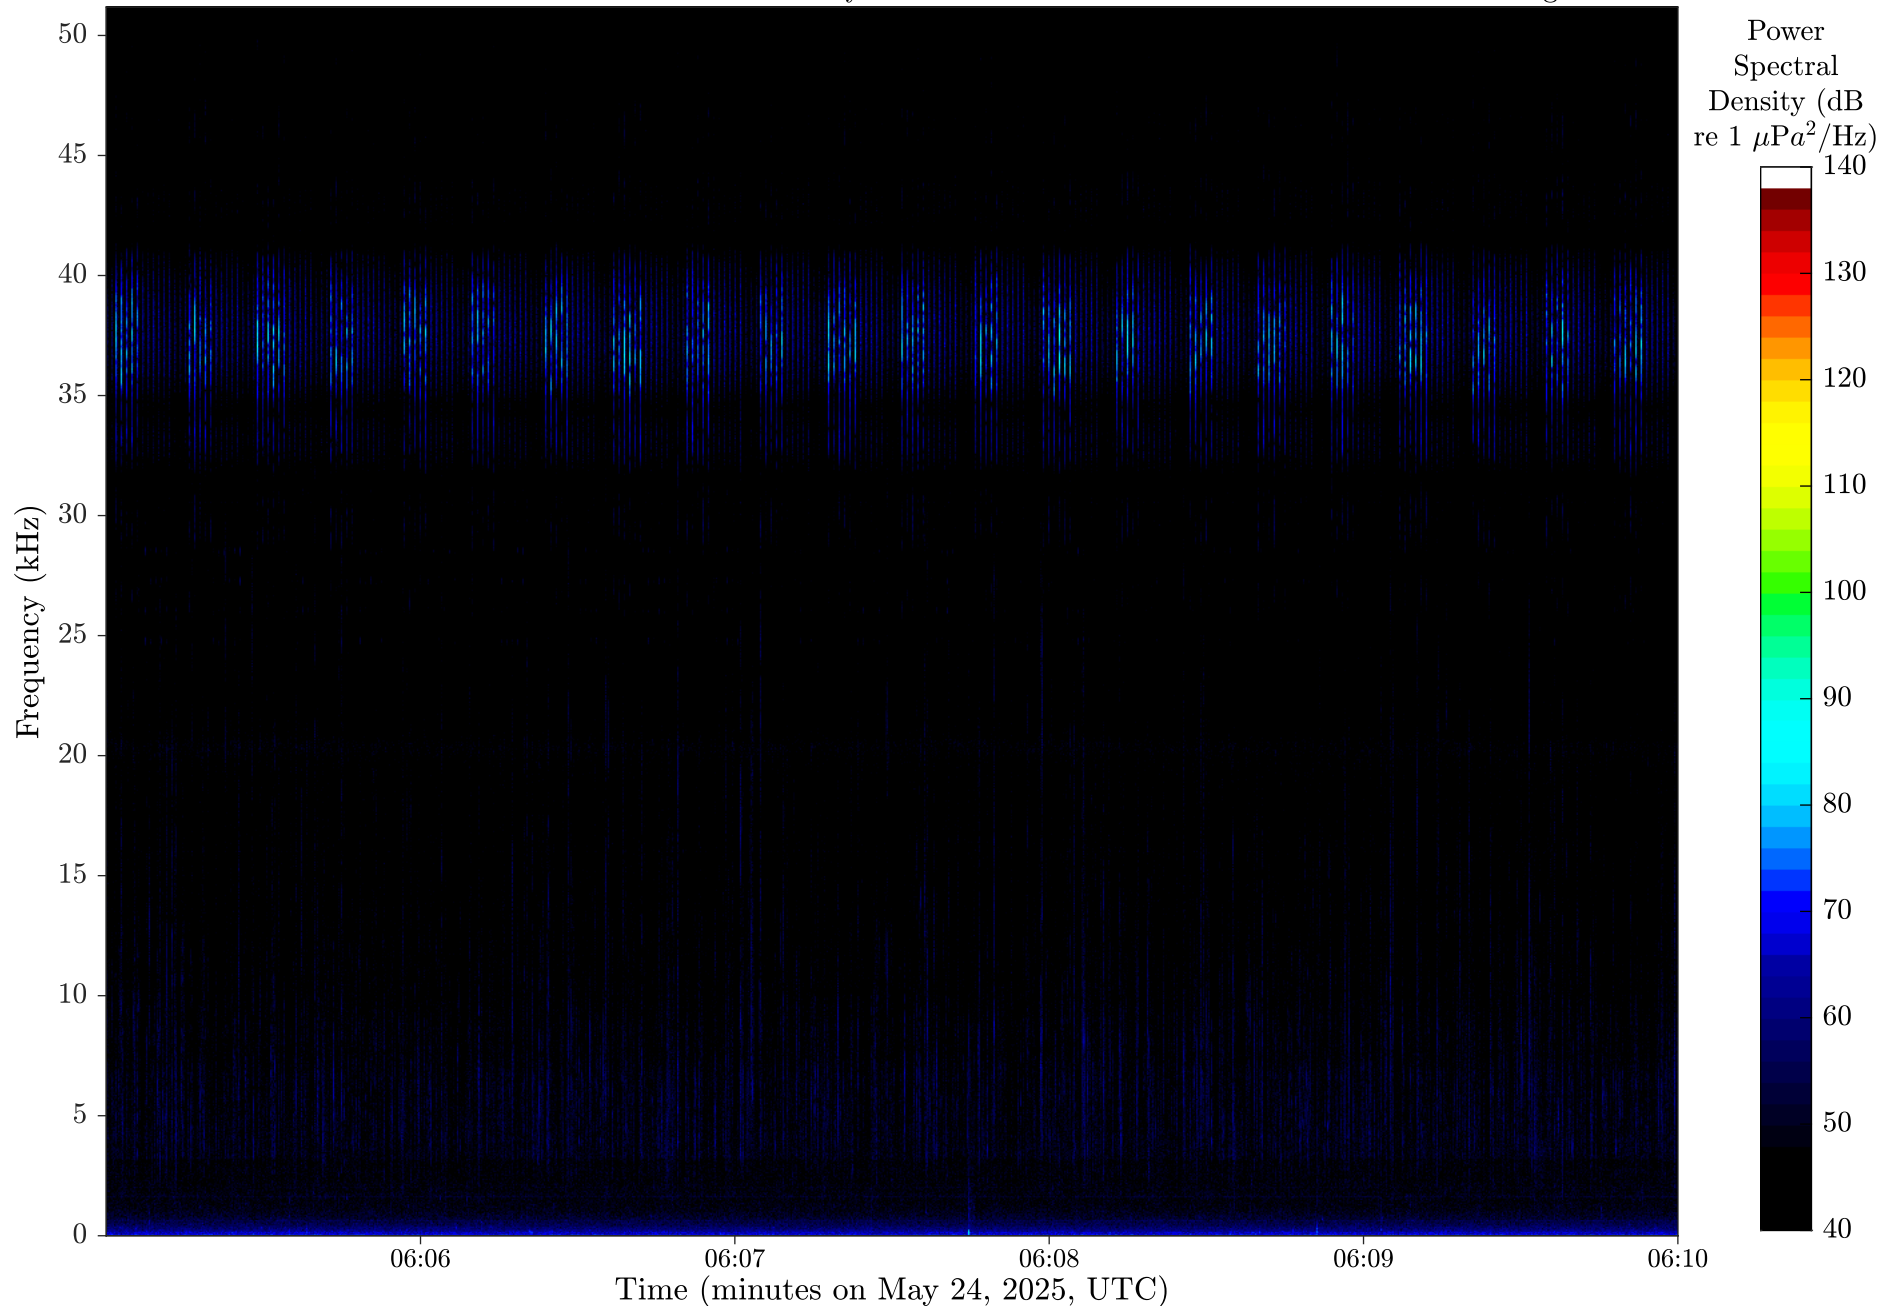



Comments: 36.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:17:26 UTC

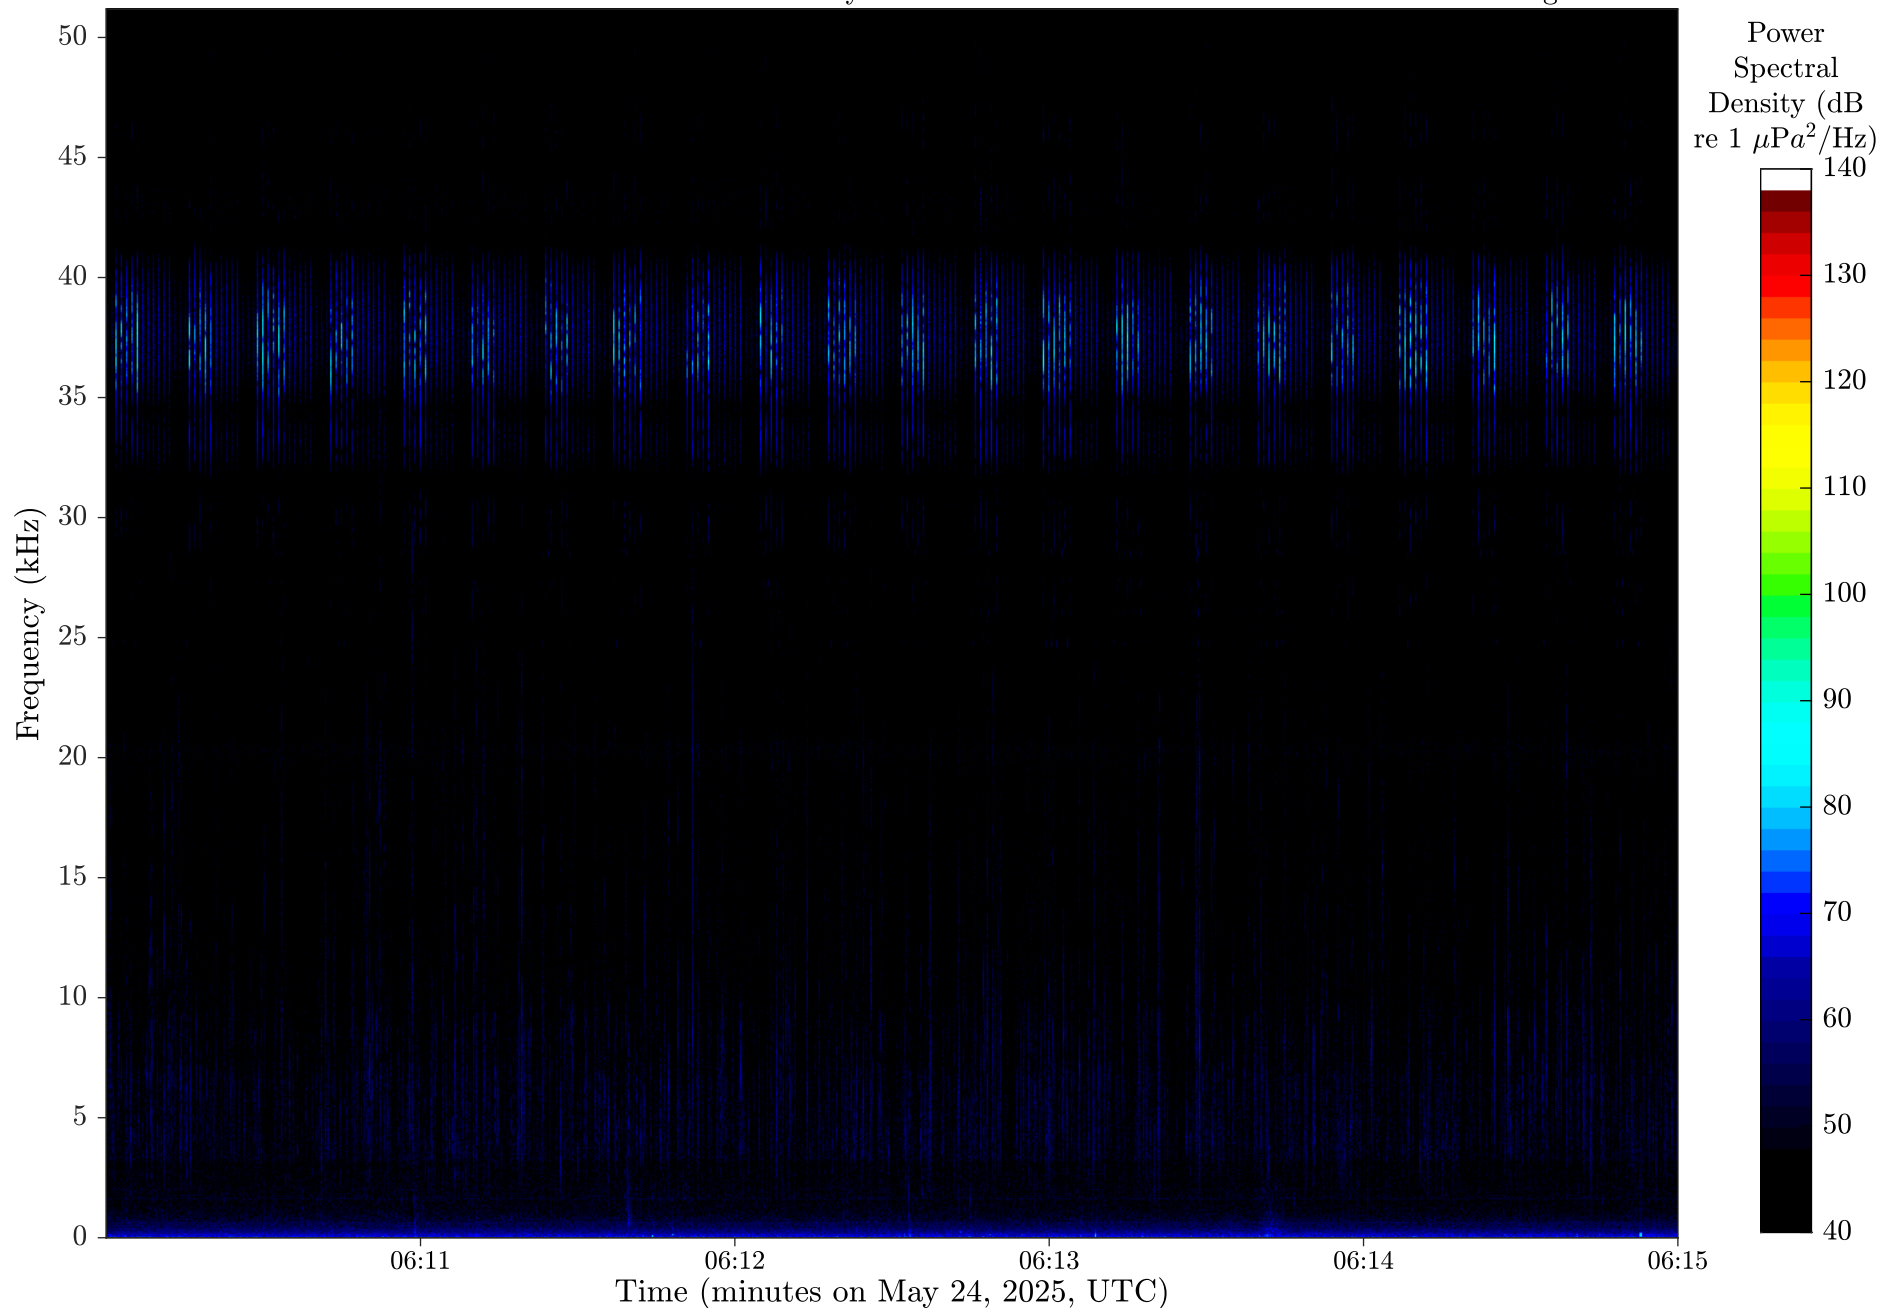

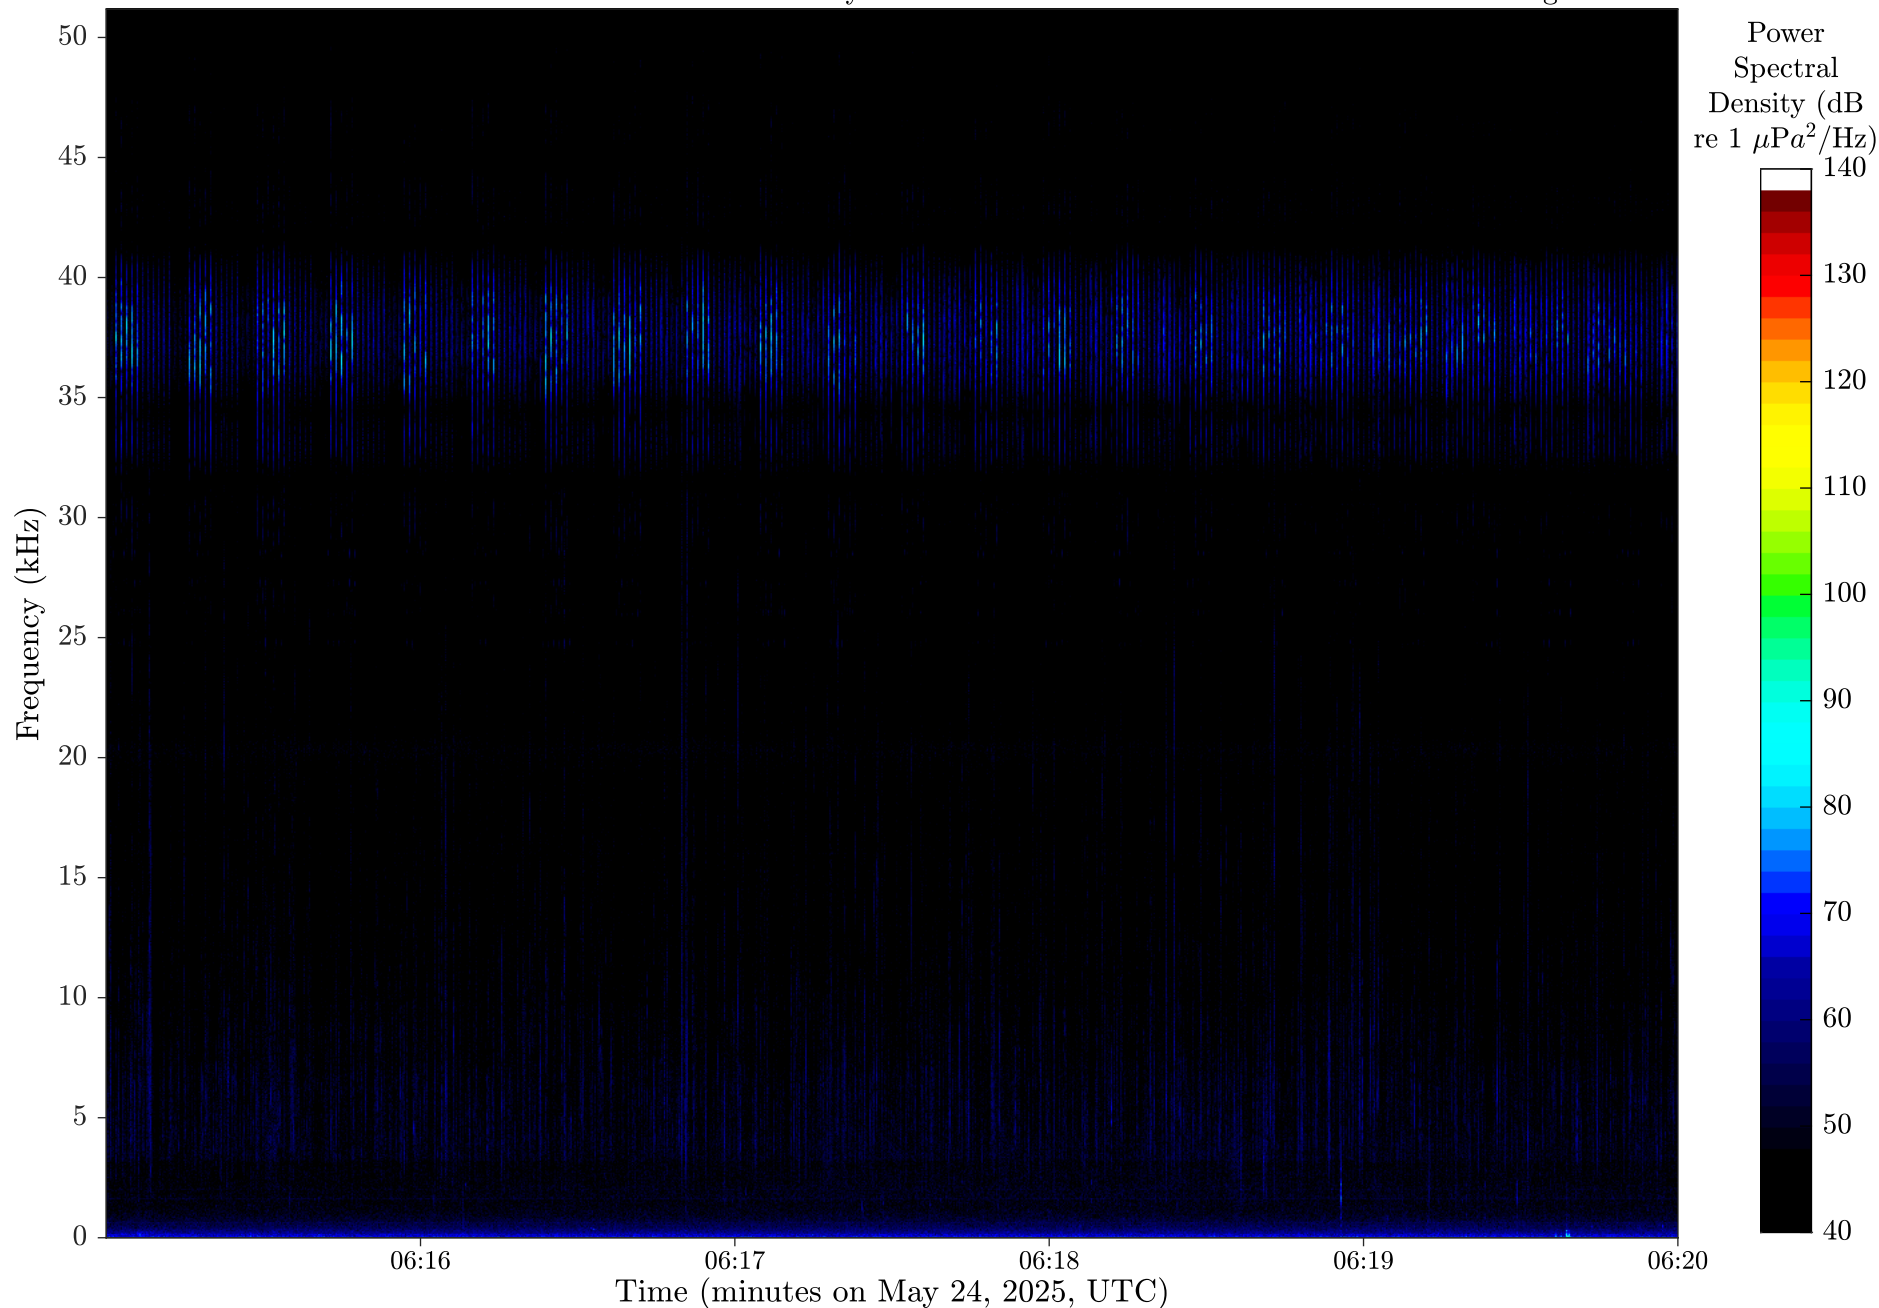


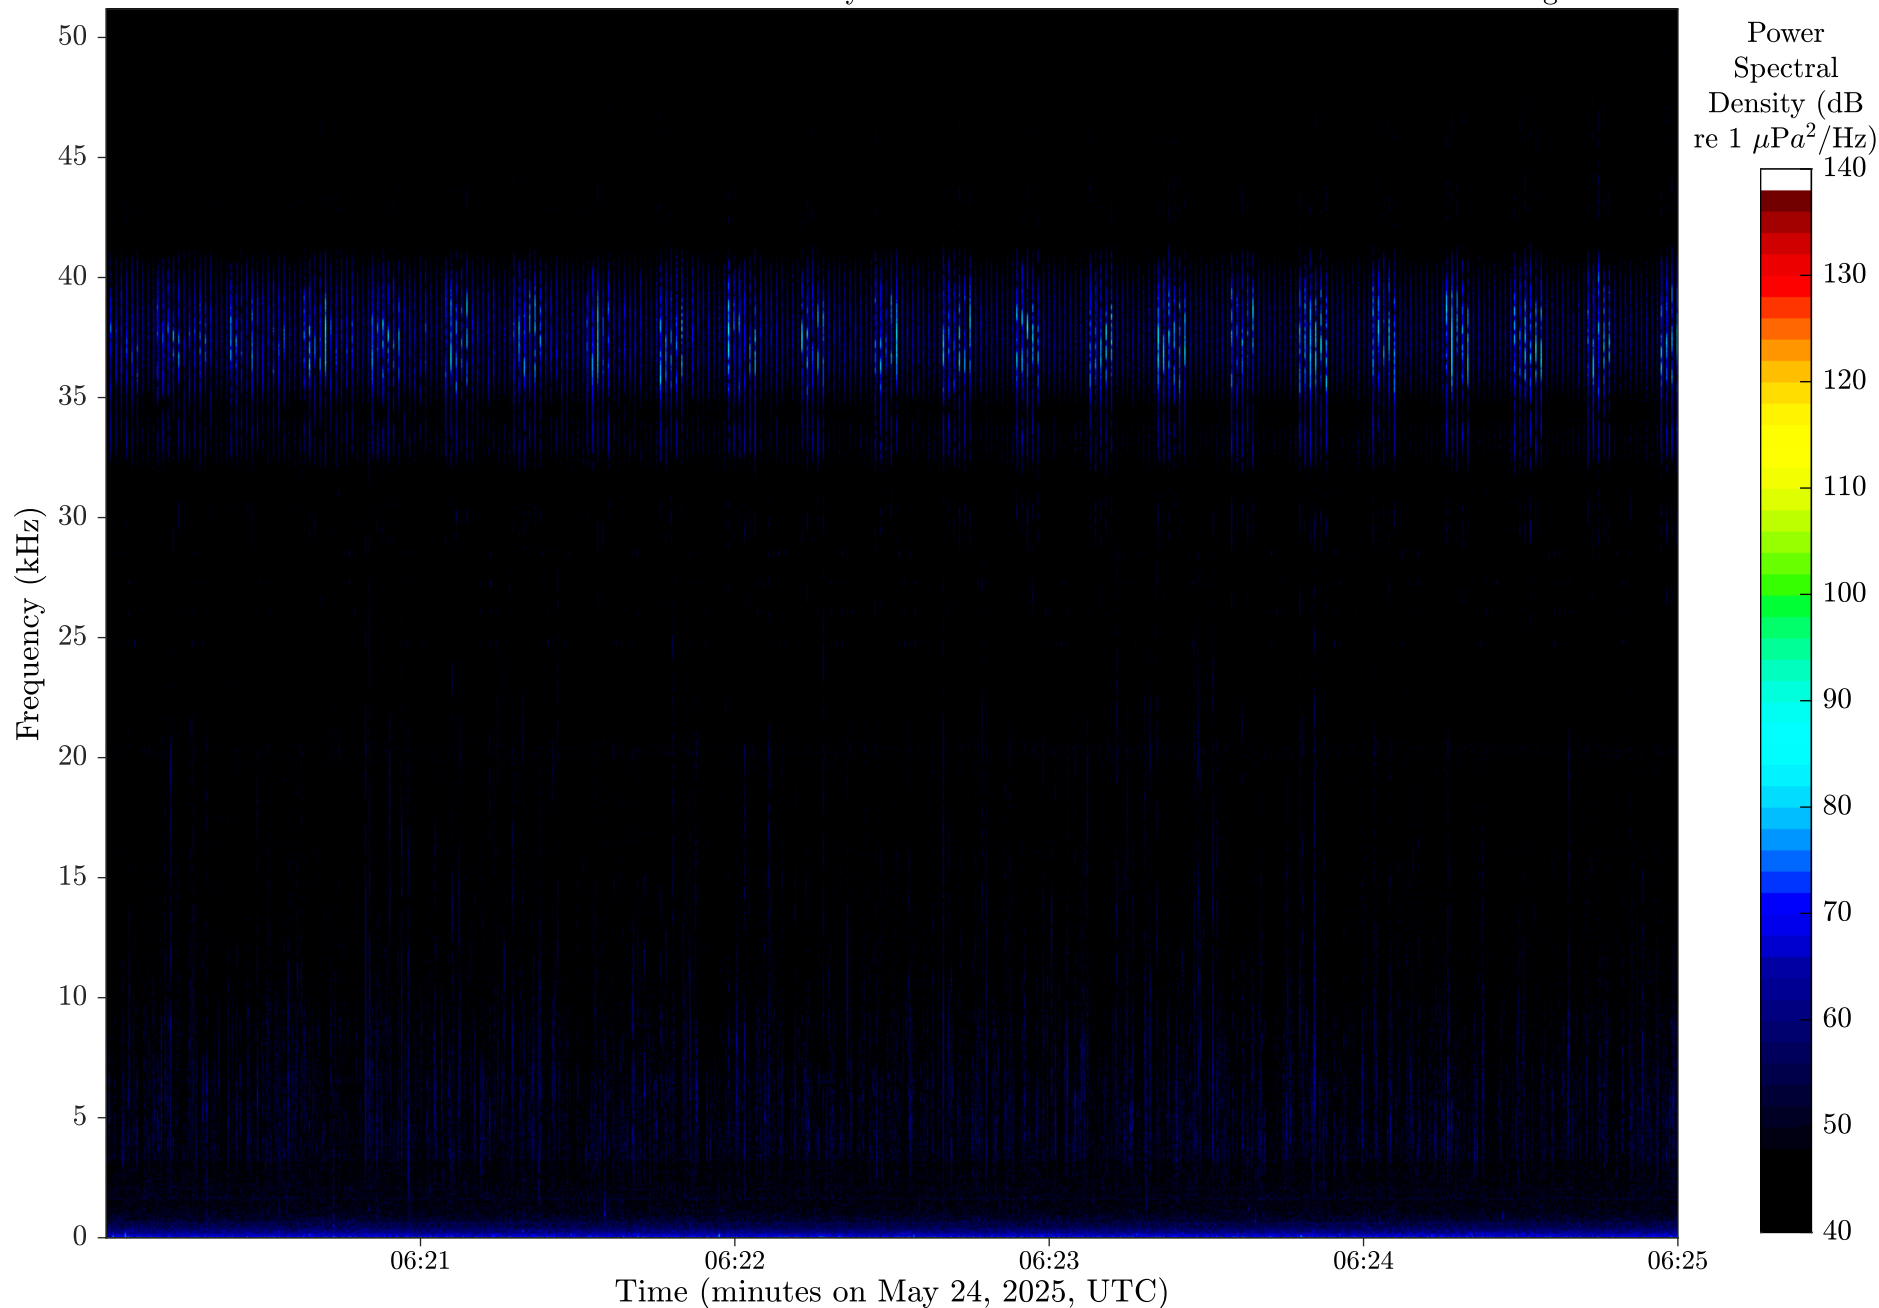

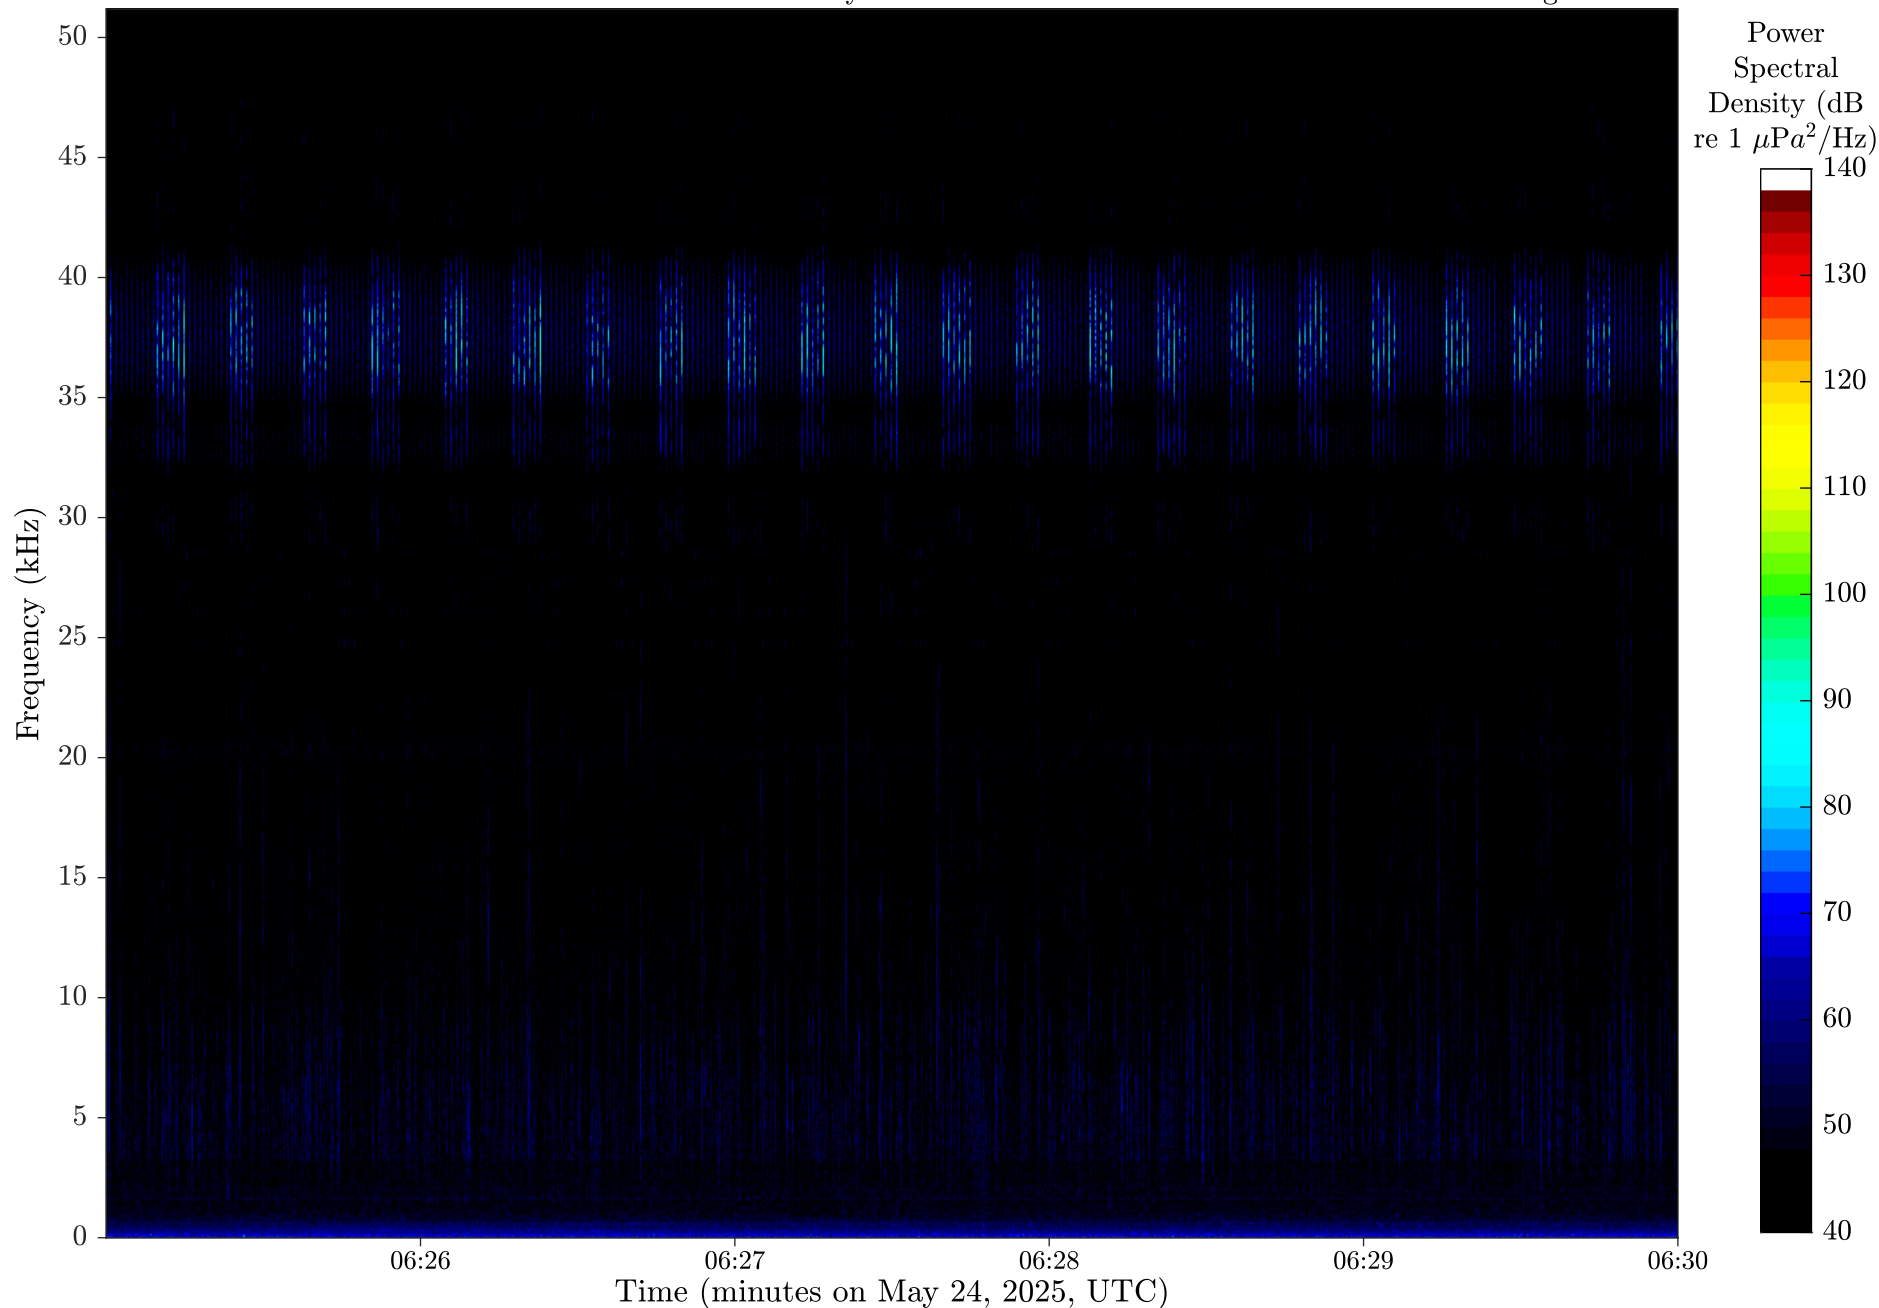


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:17:59 UTC

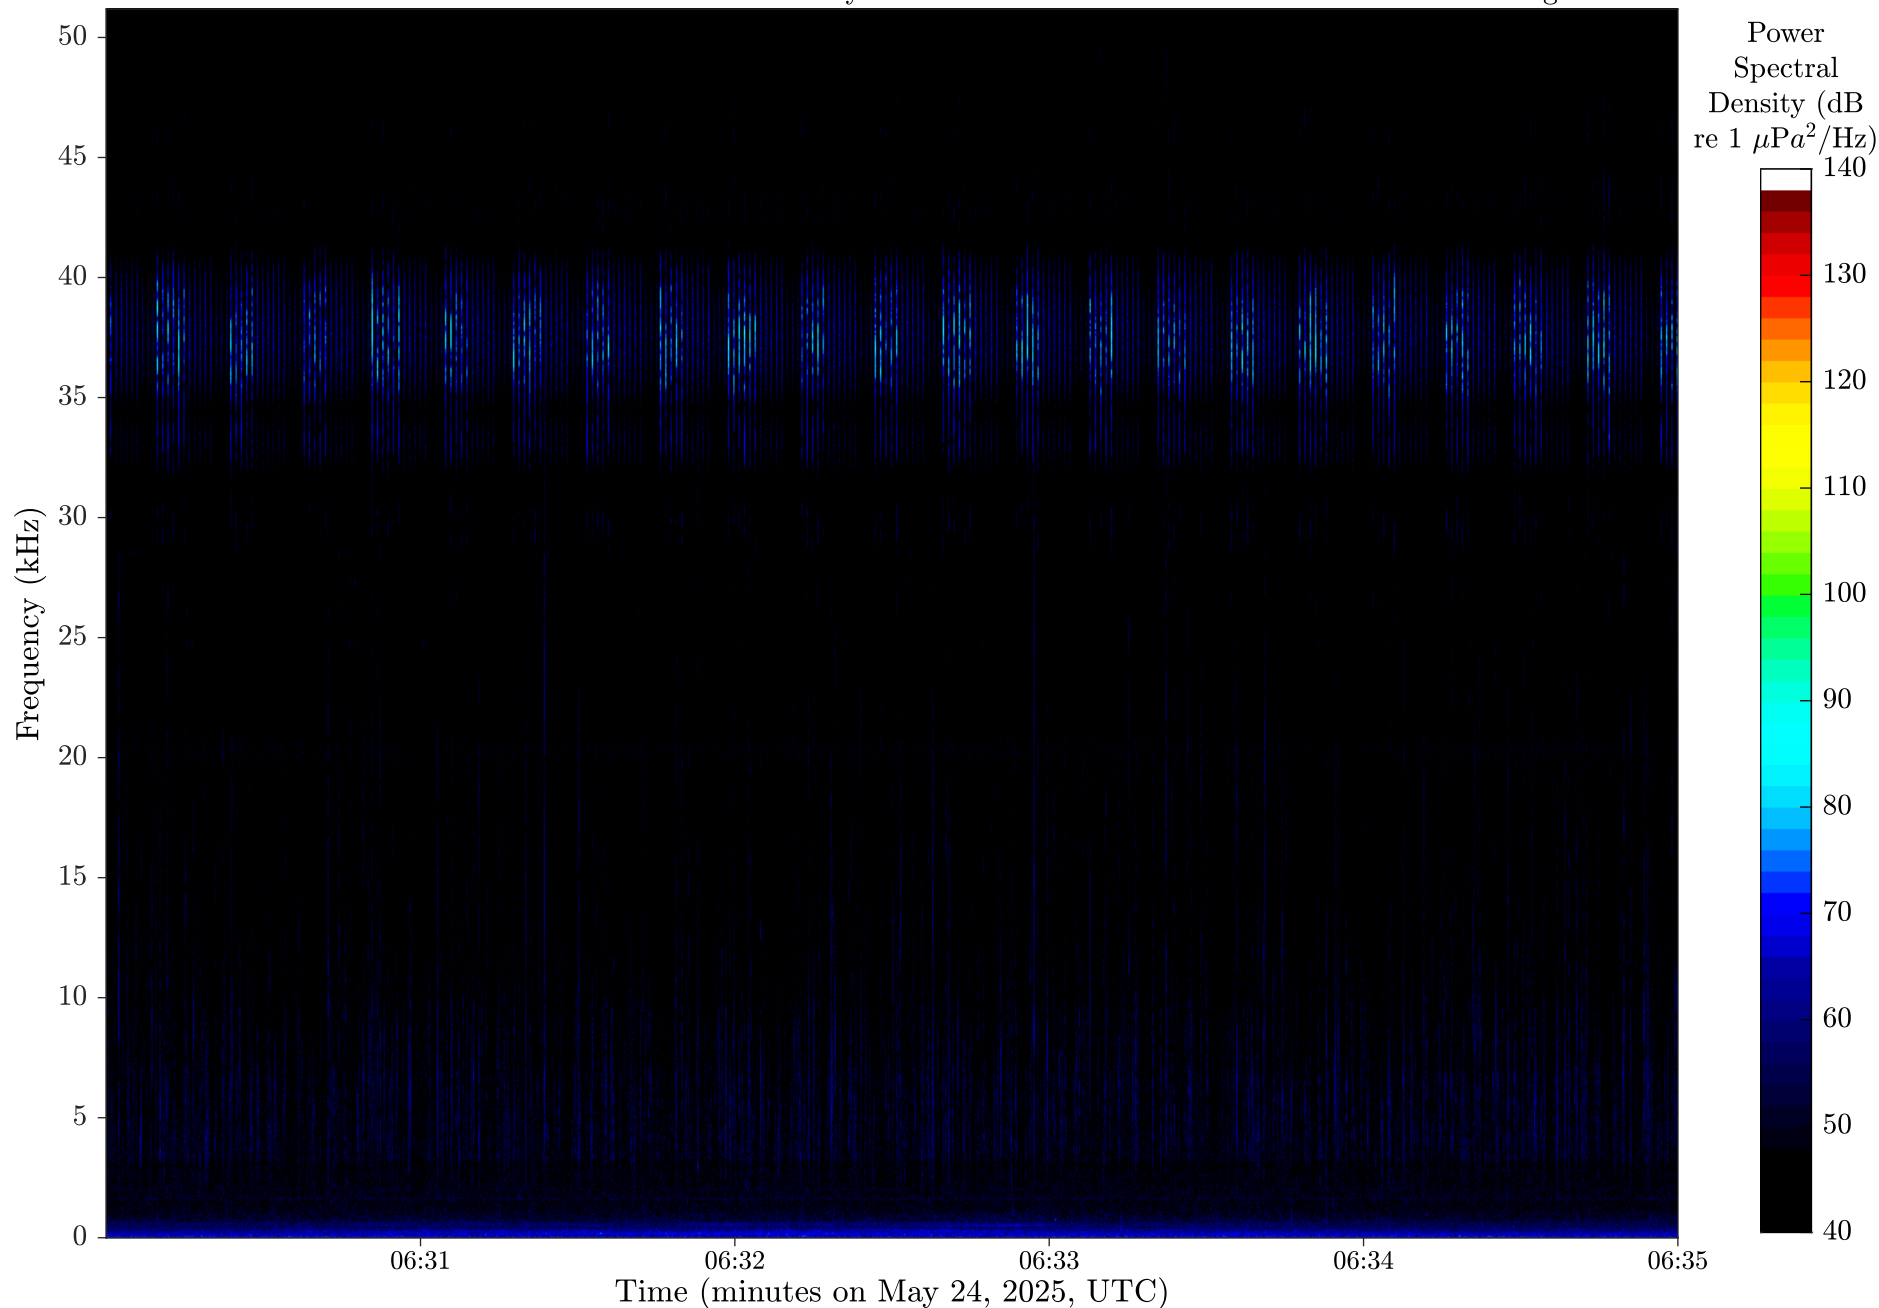


Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:18:07 UTC

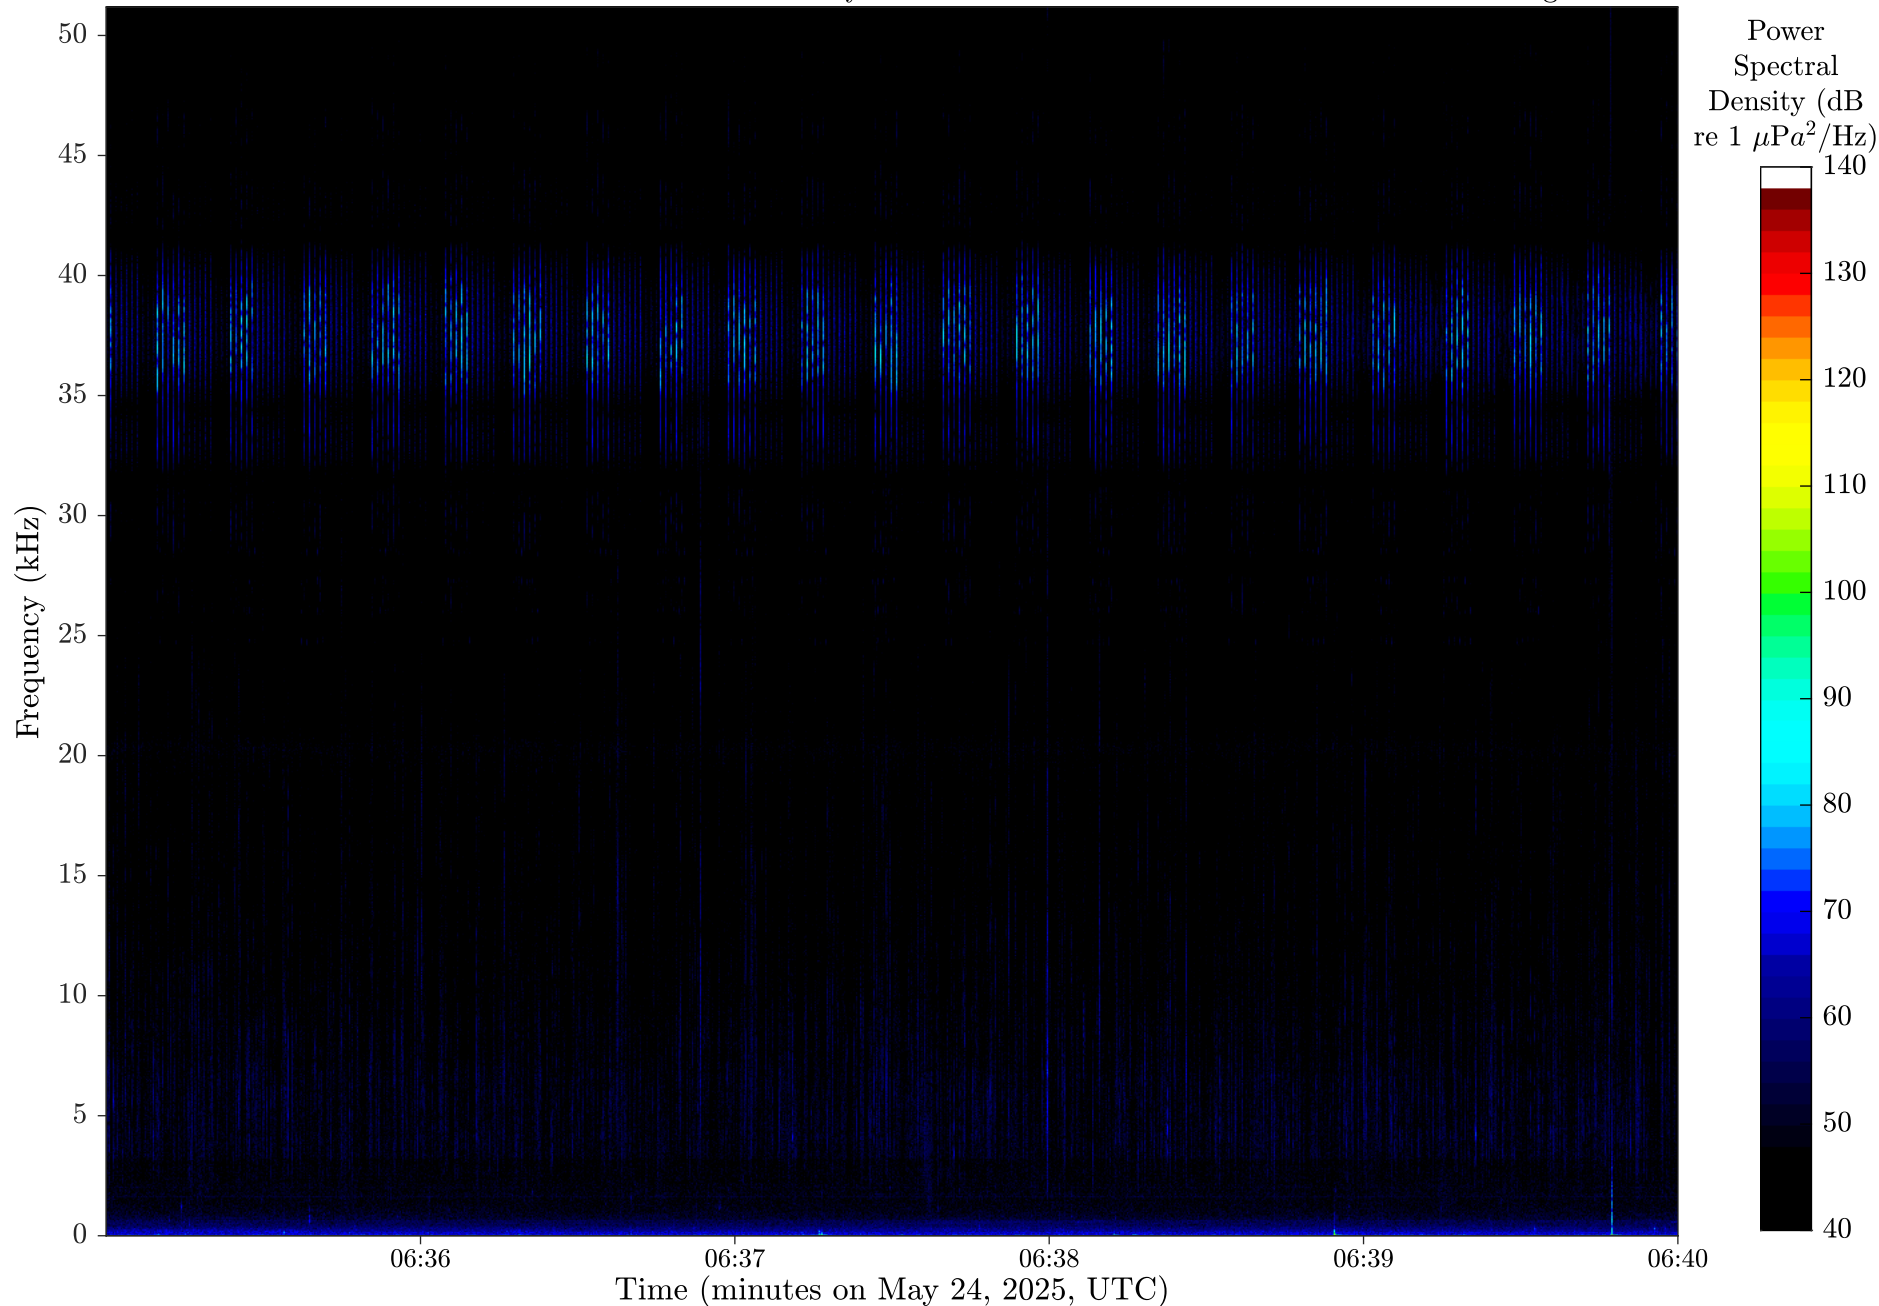


Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:18:15 UTC

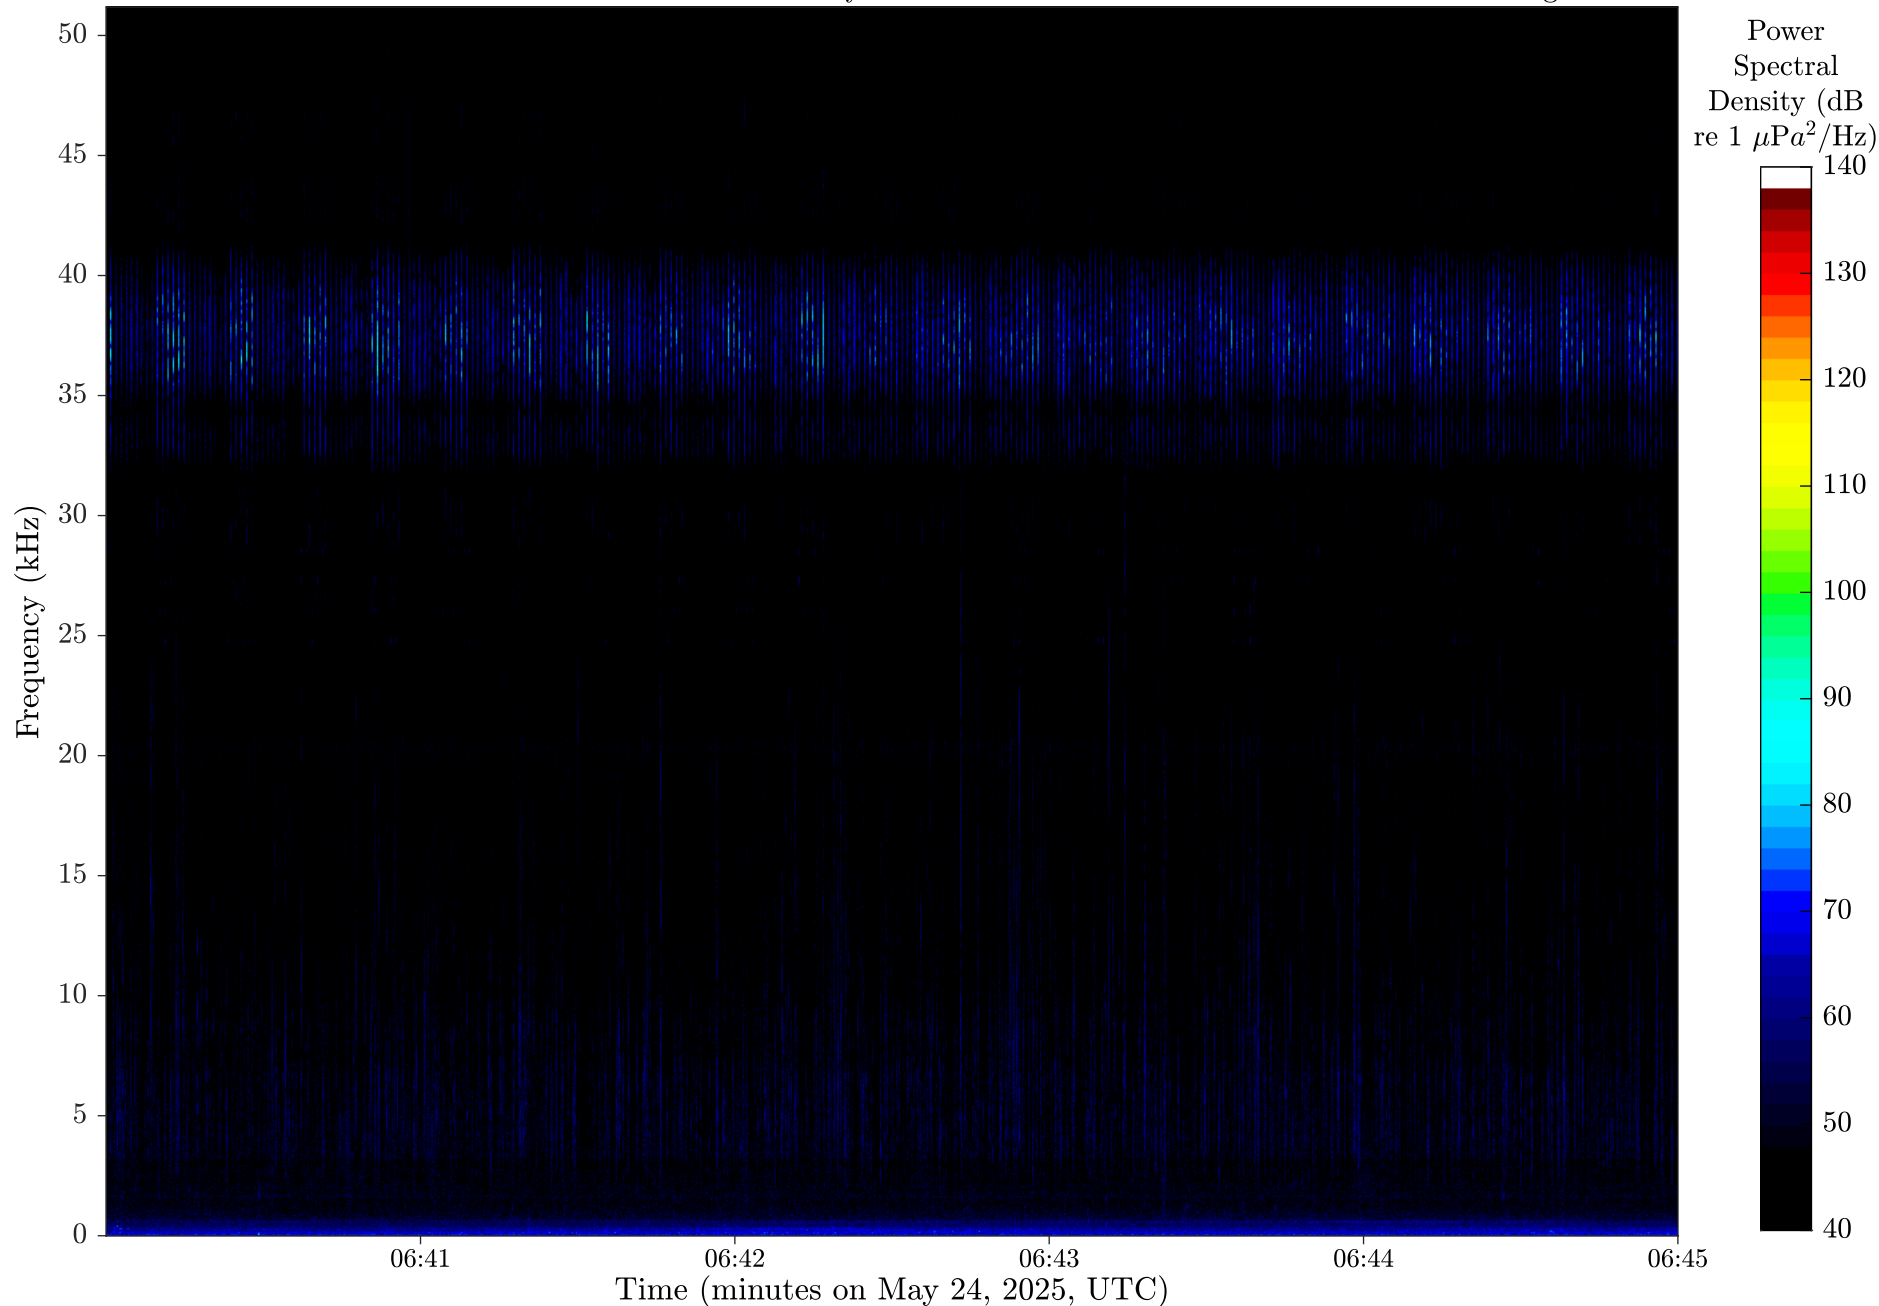


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:18:22 UTC

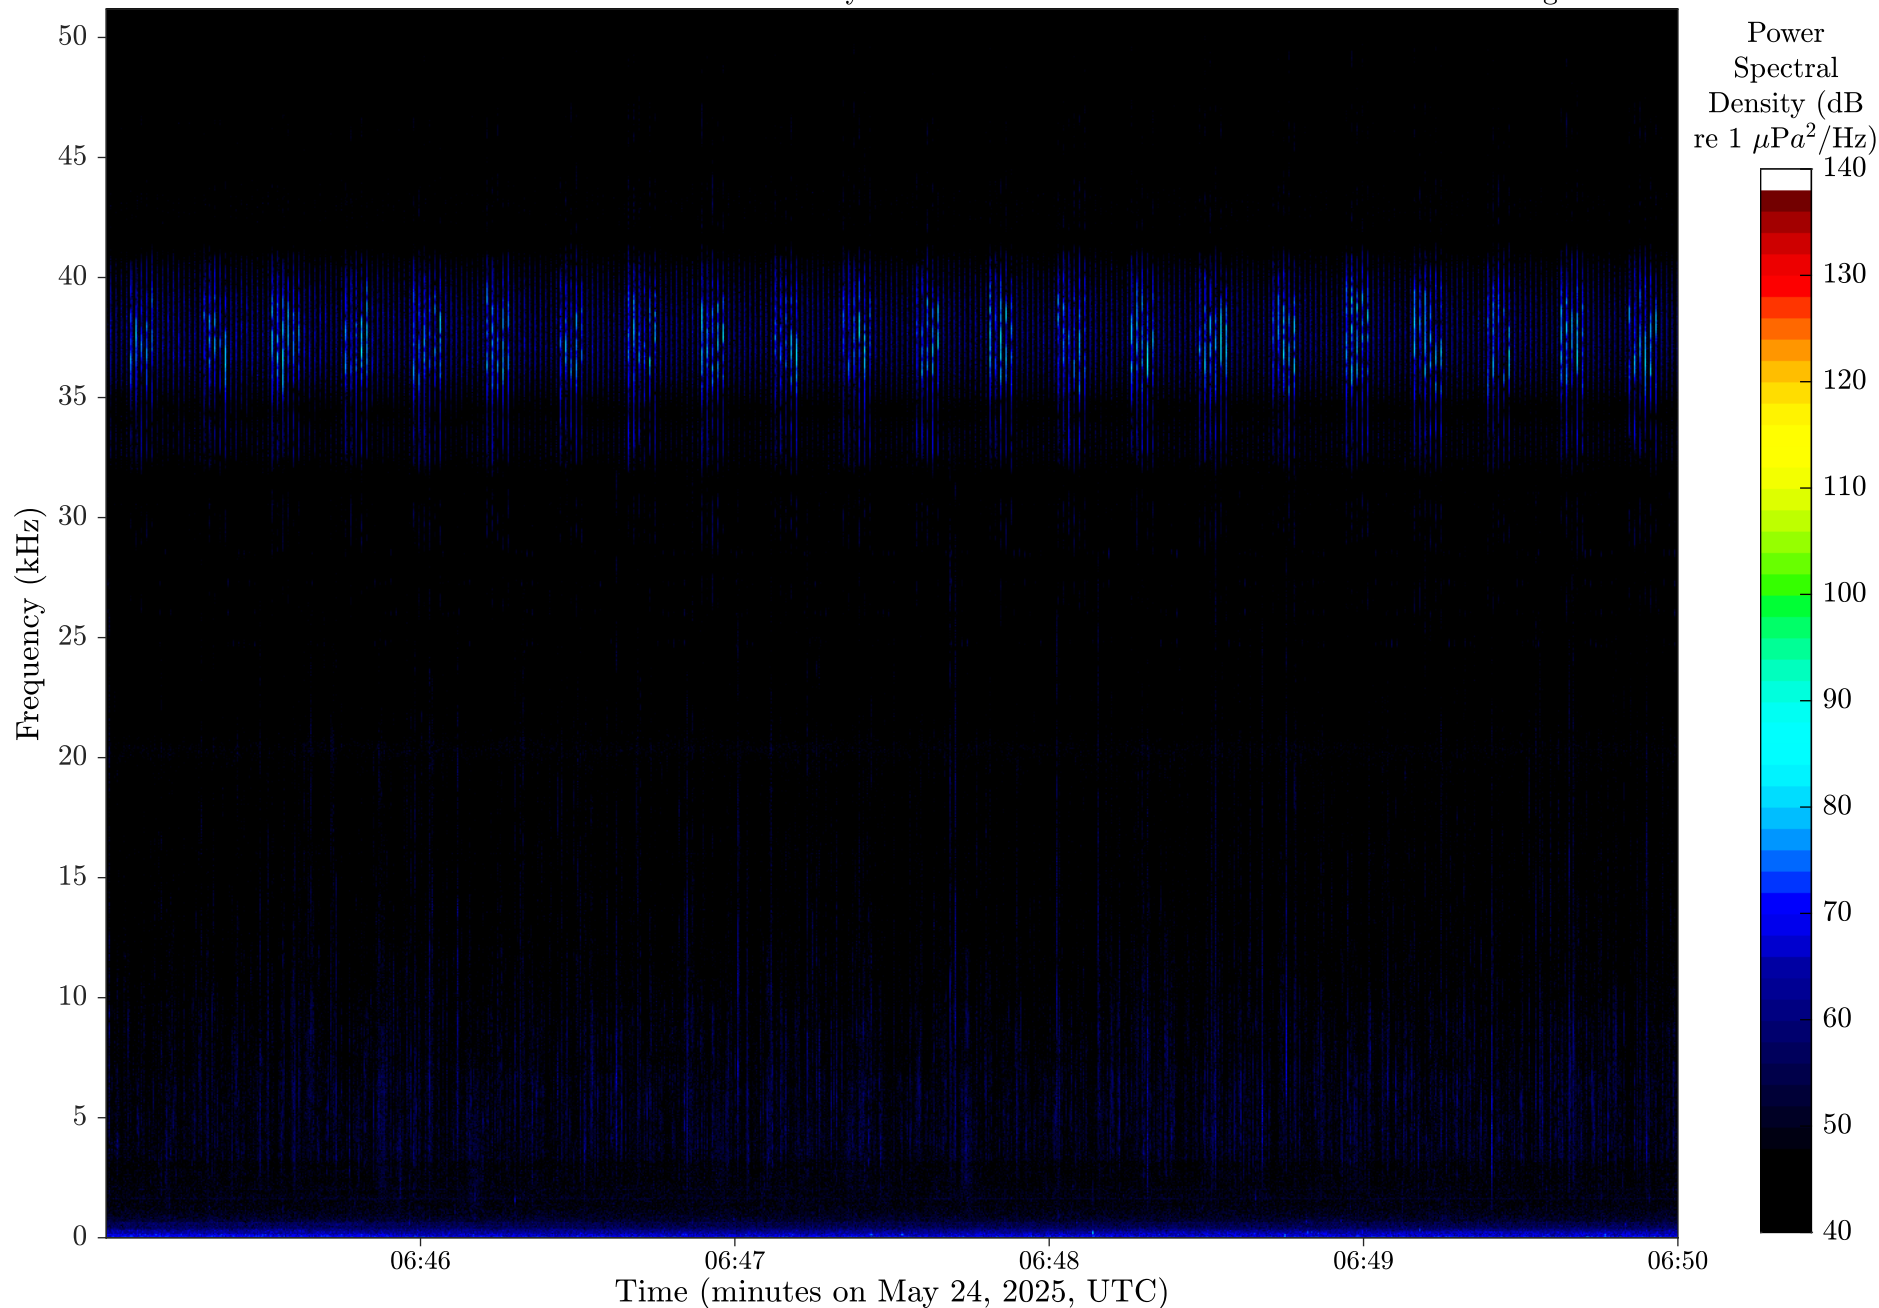


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:18:30 UTC

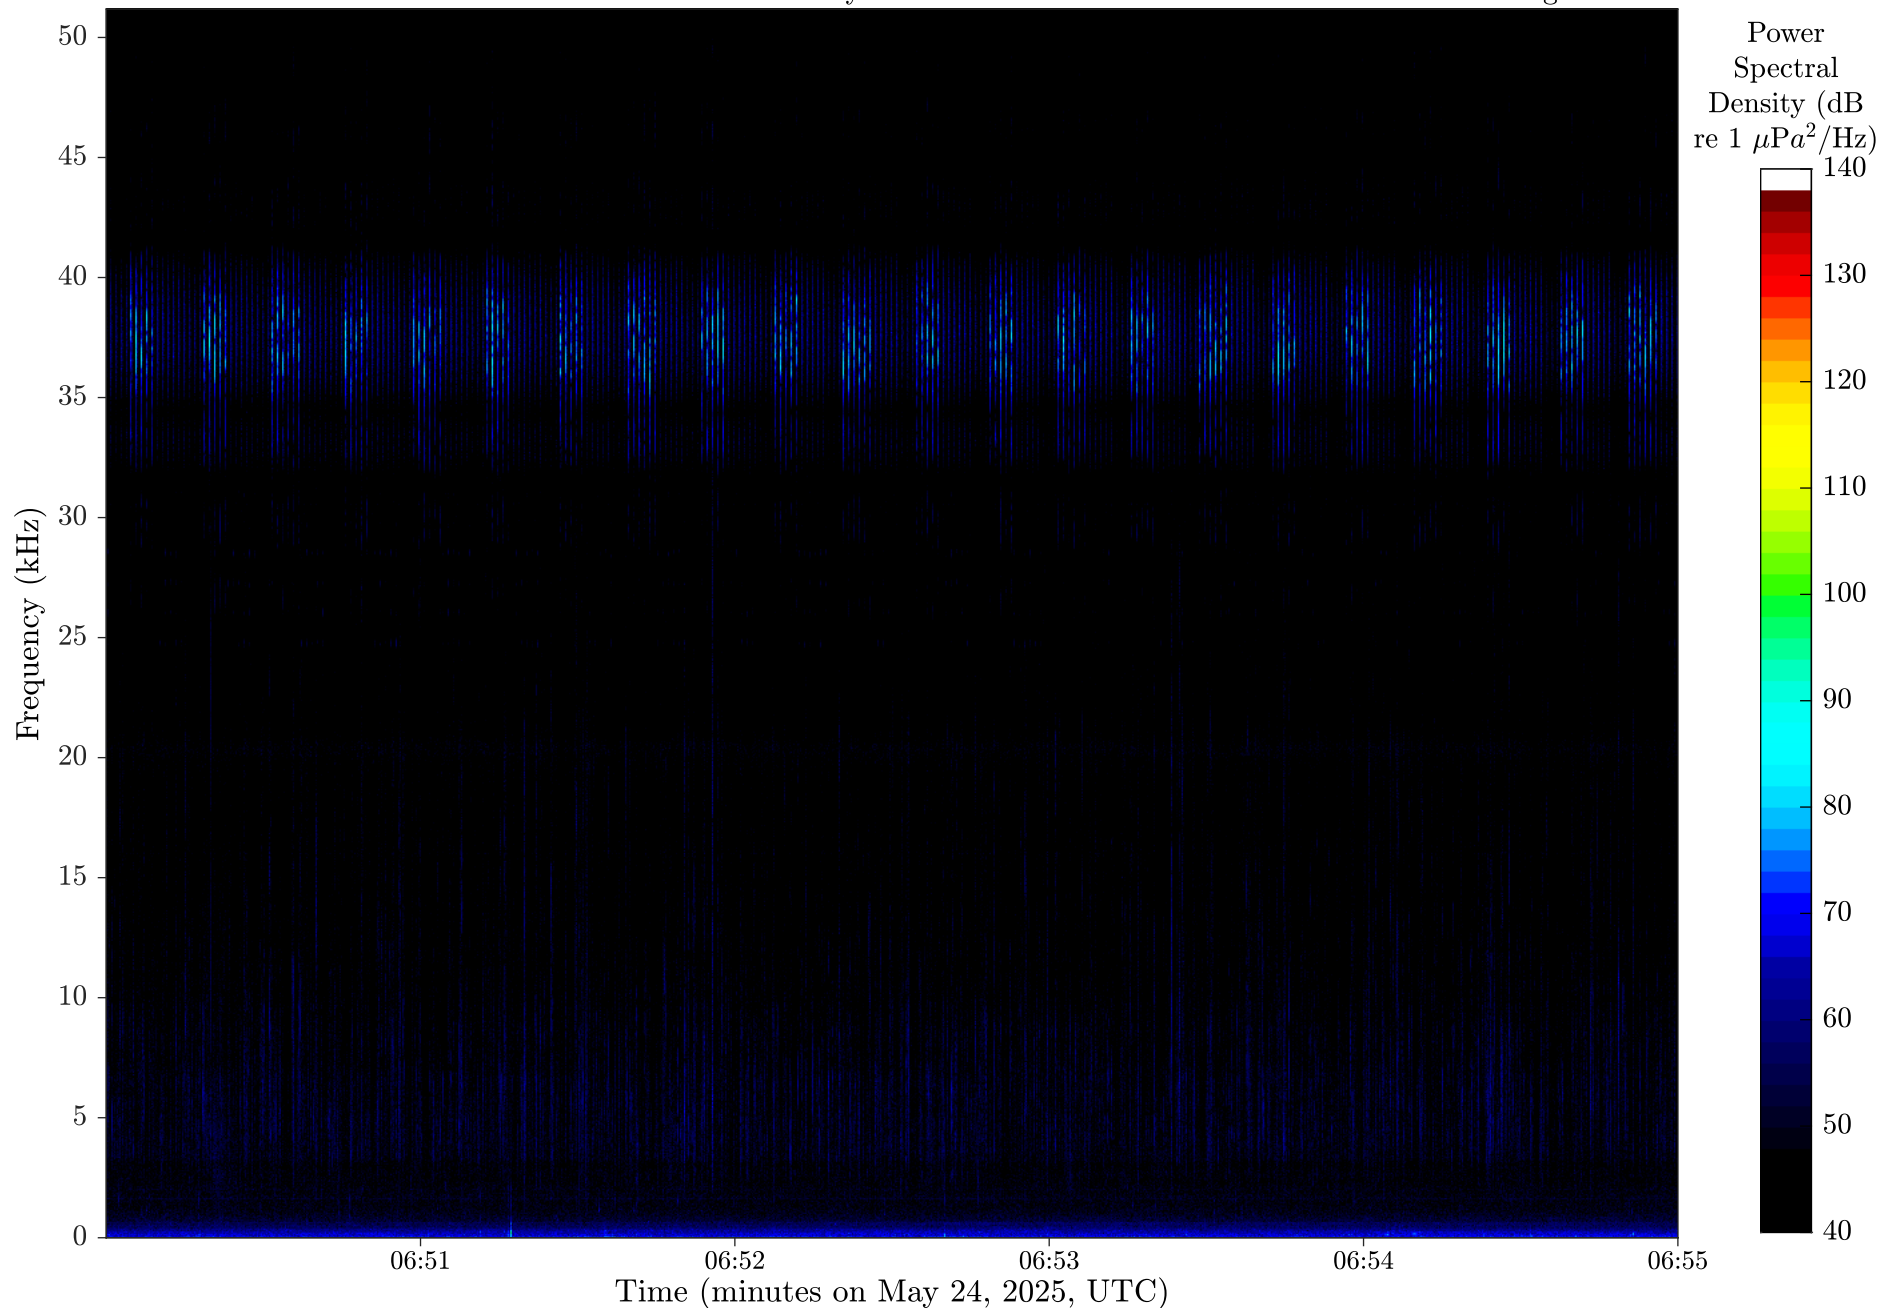


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:18:37 UTC

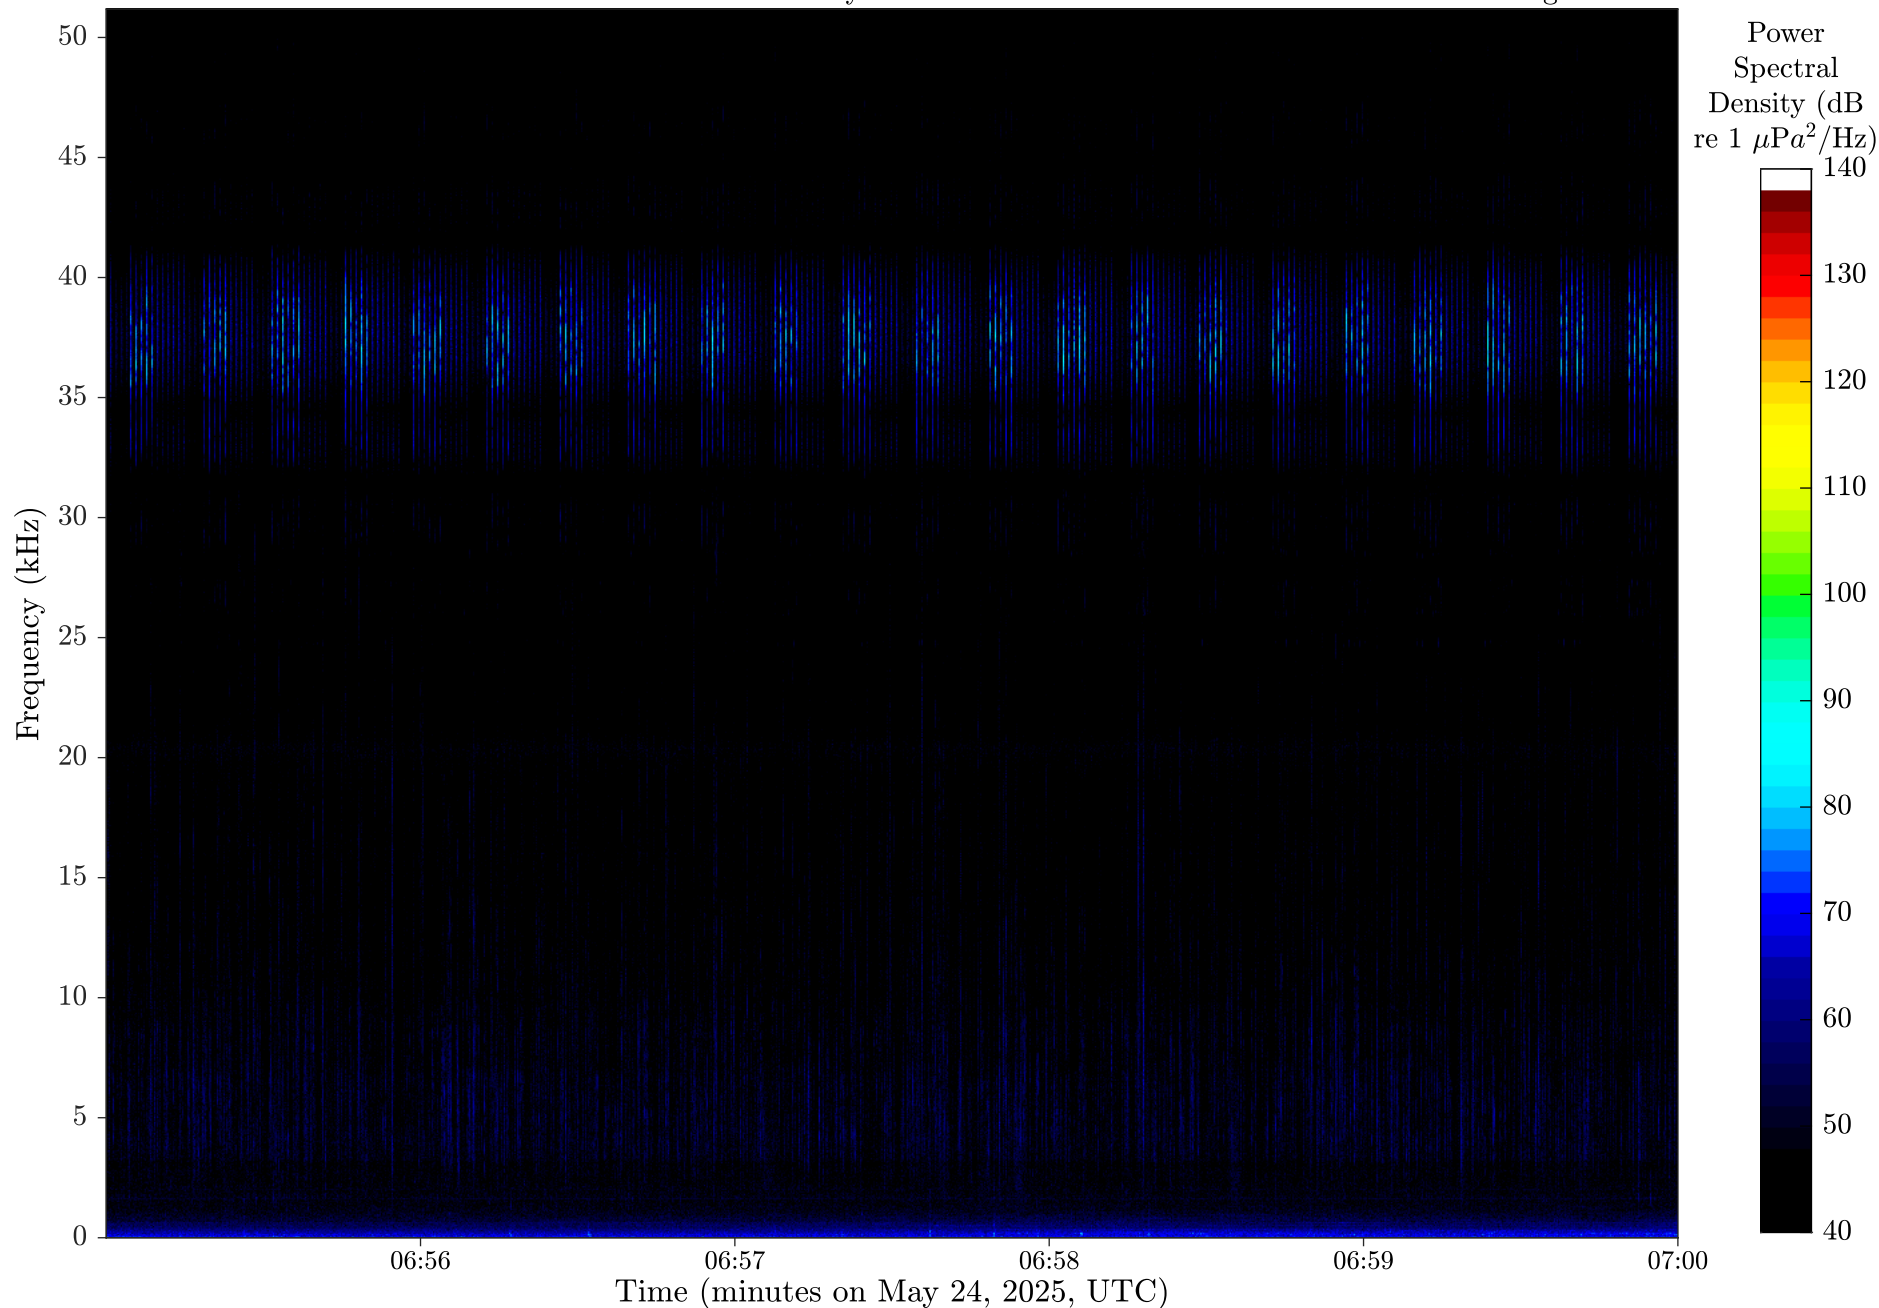

Comments: 36.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:18:45 UTC

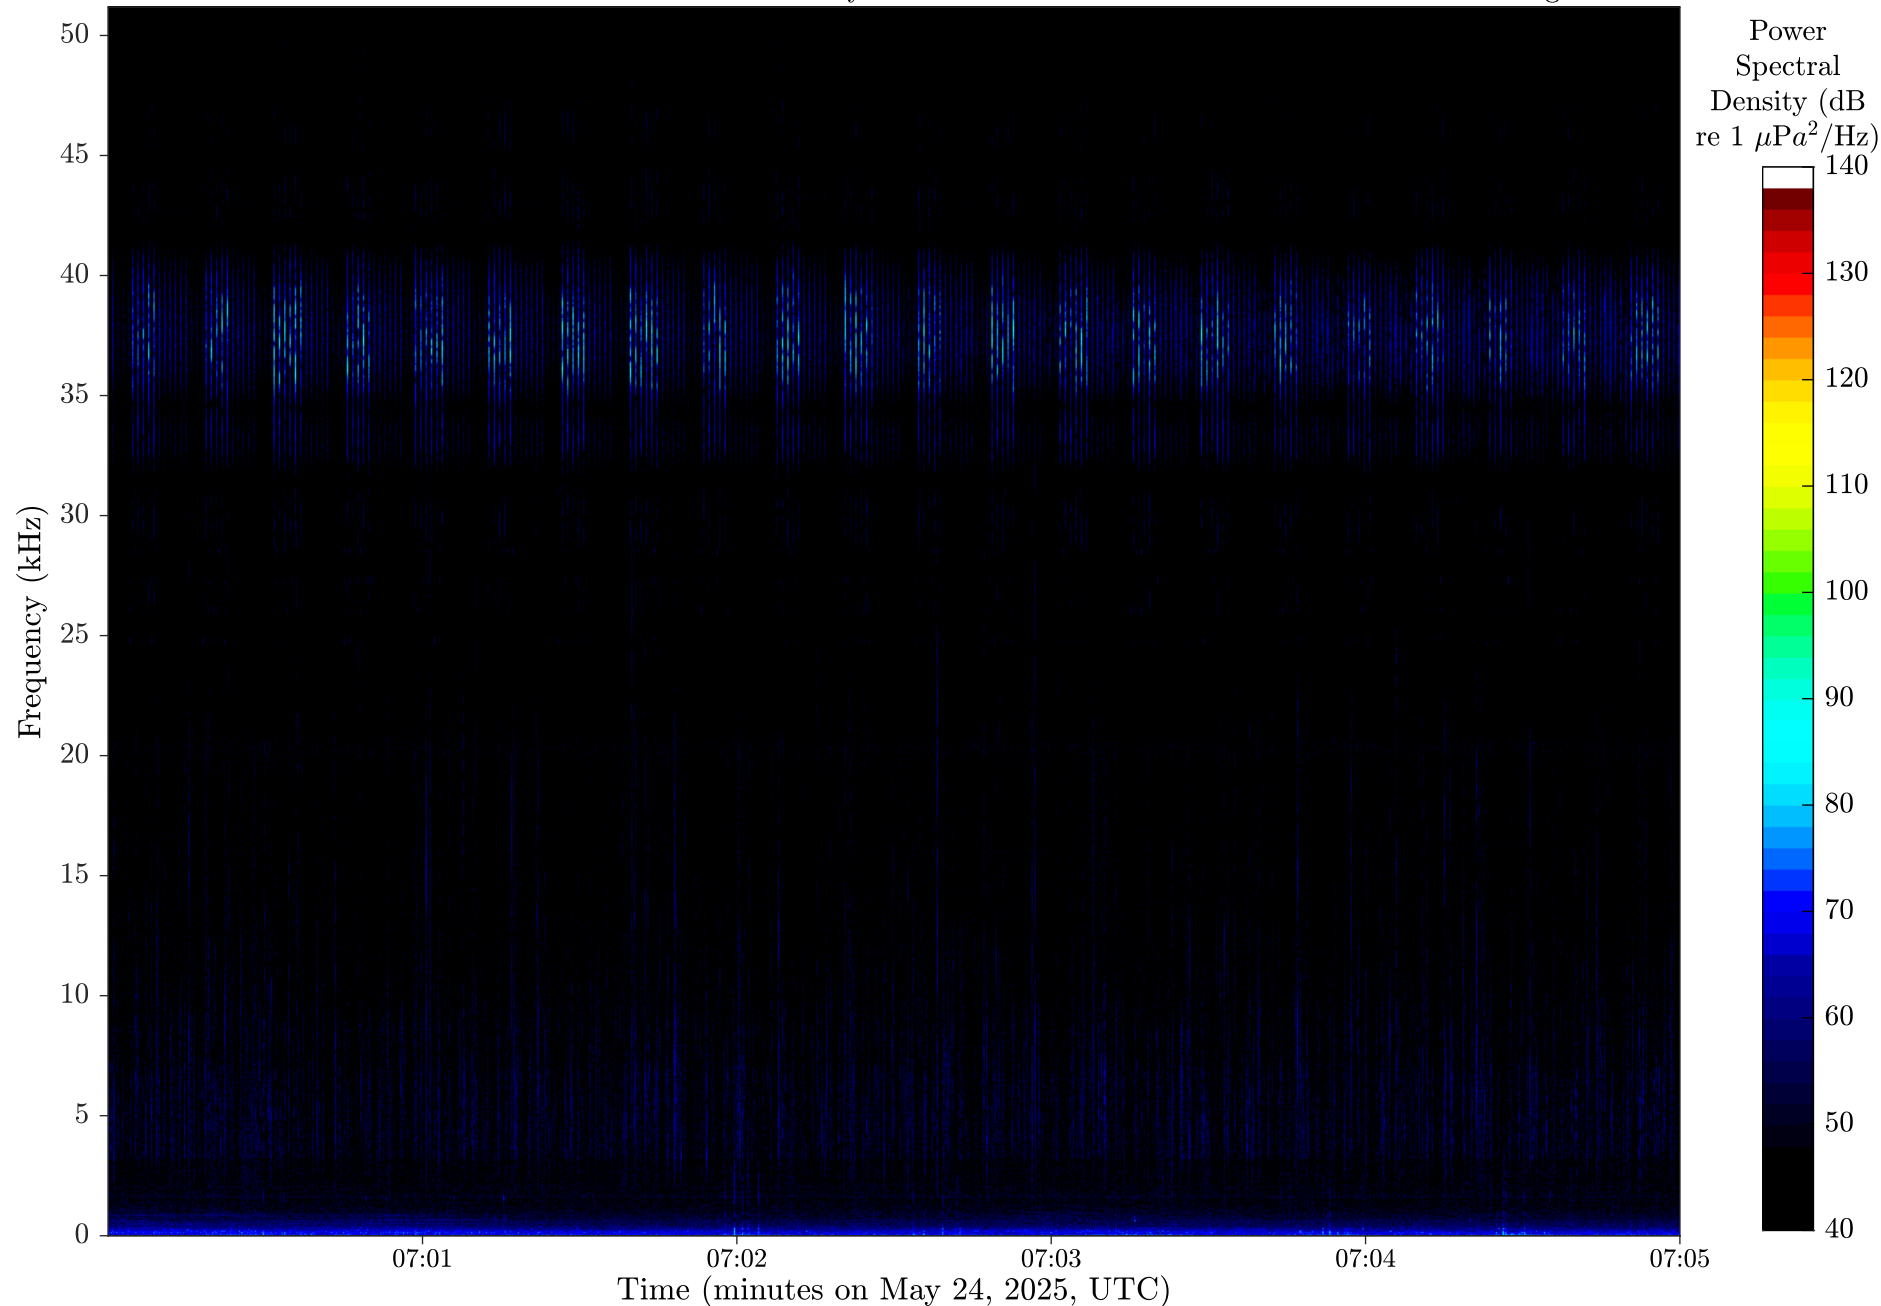


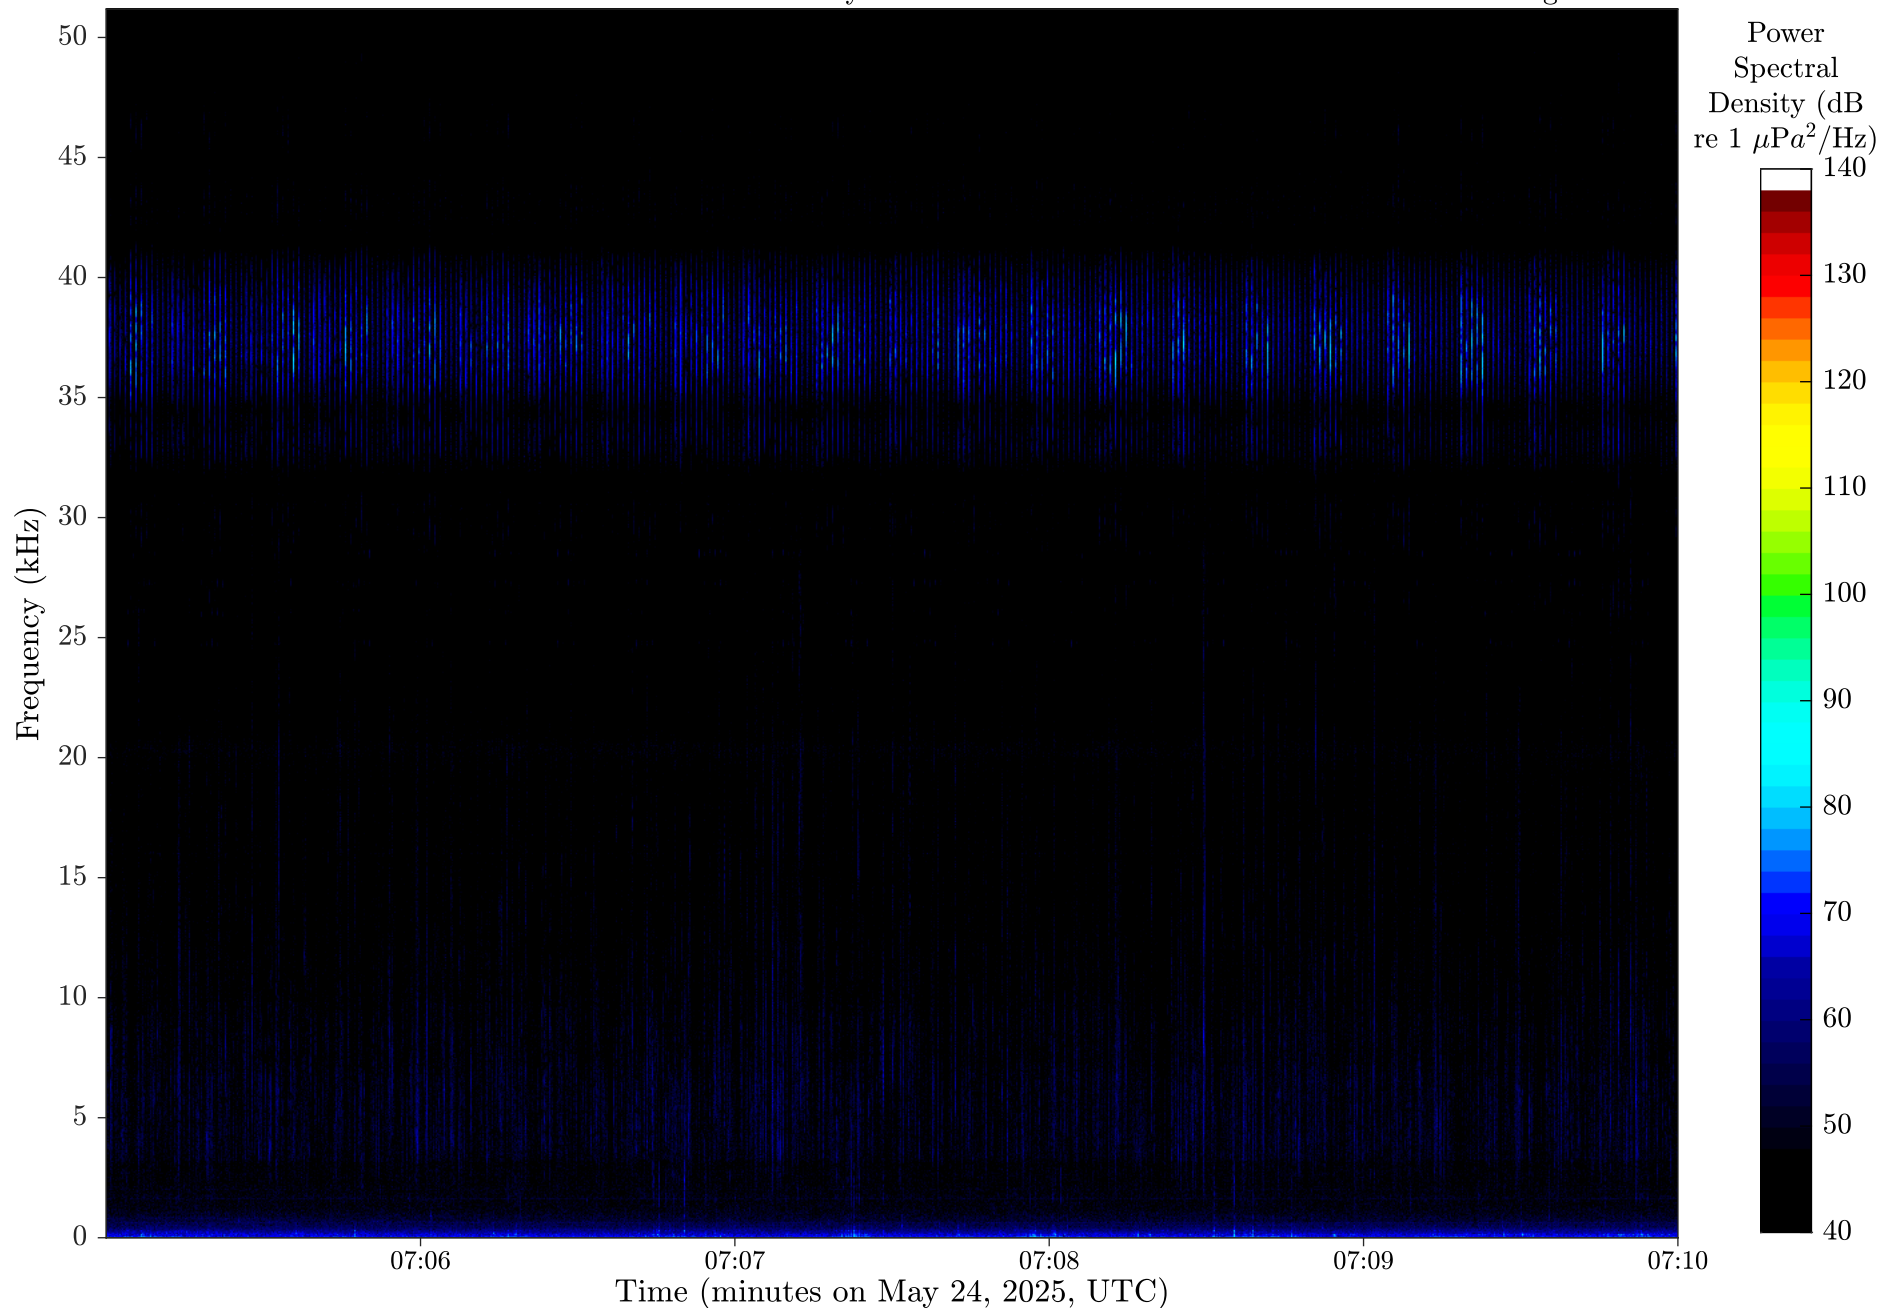


Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:18:59 UTC

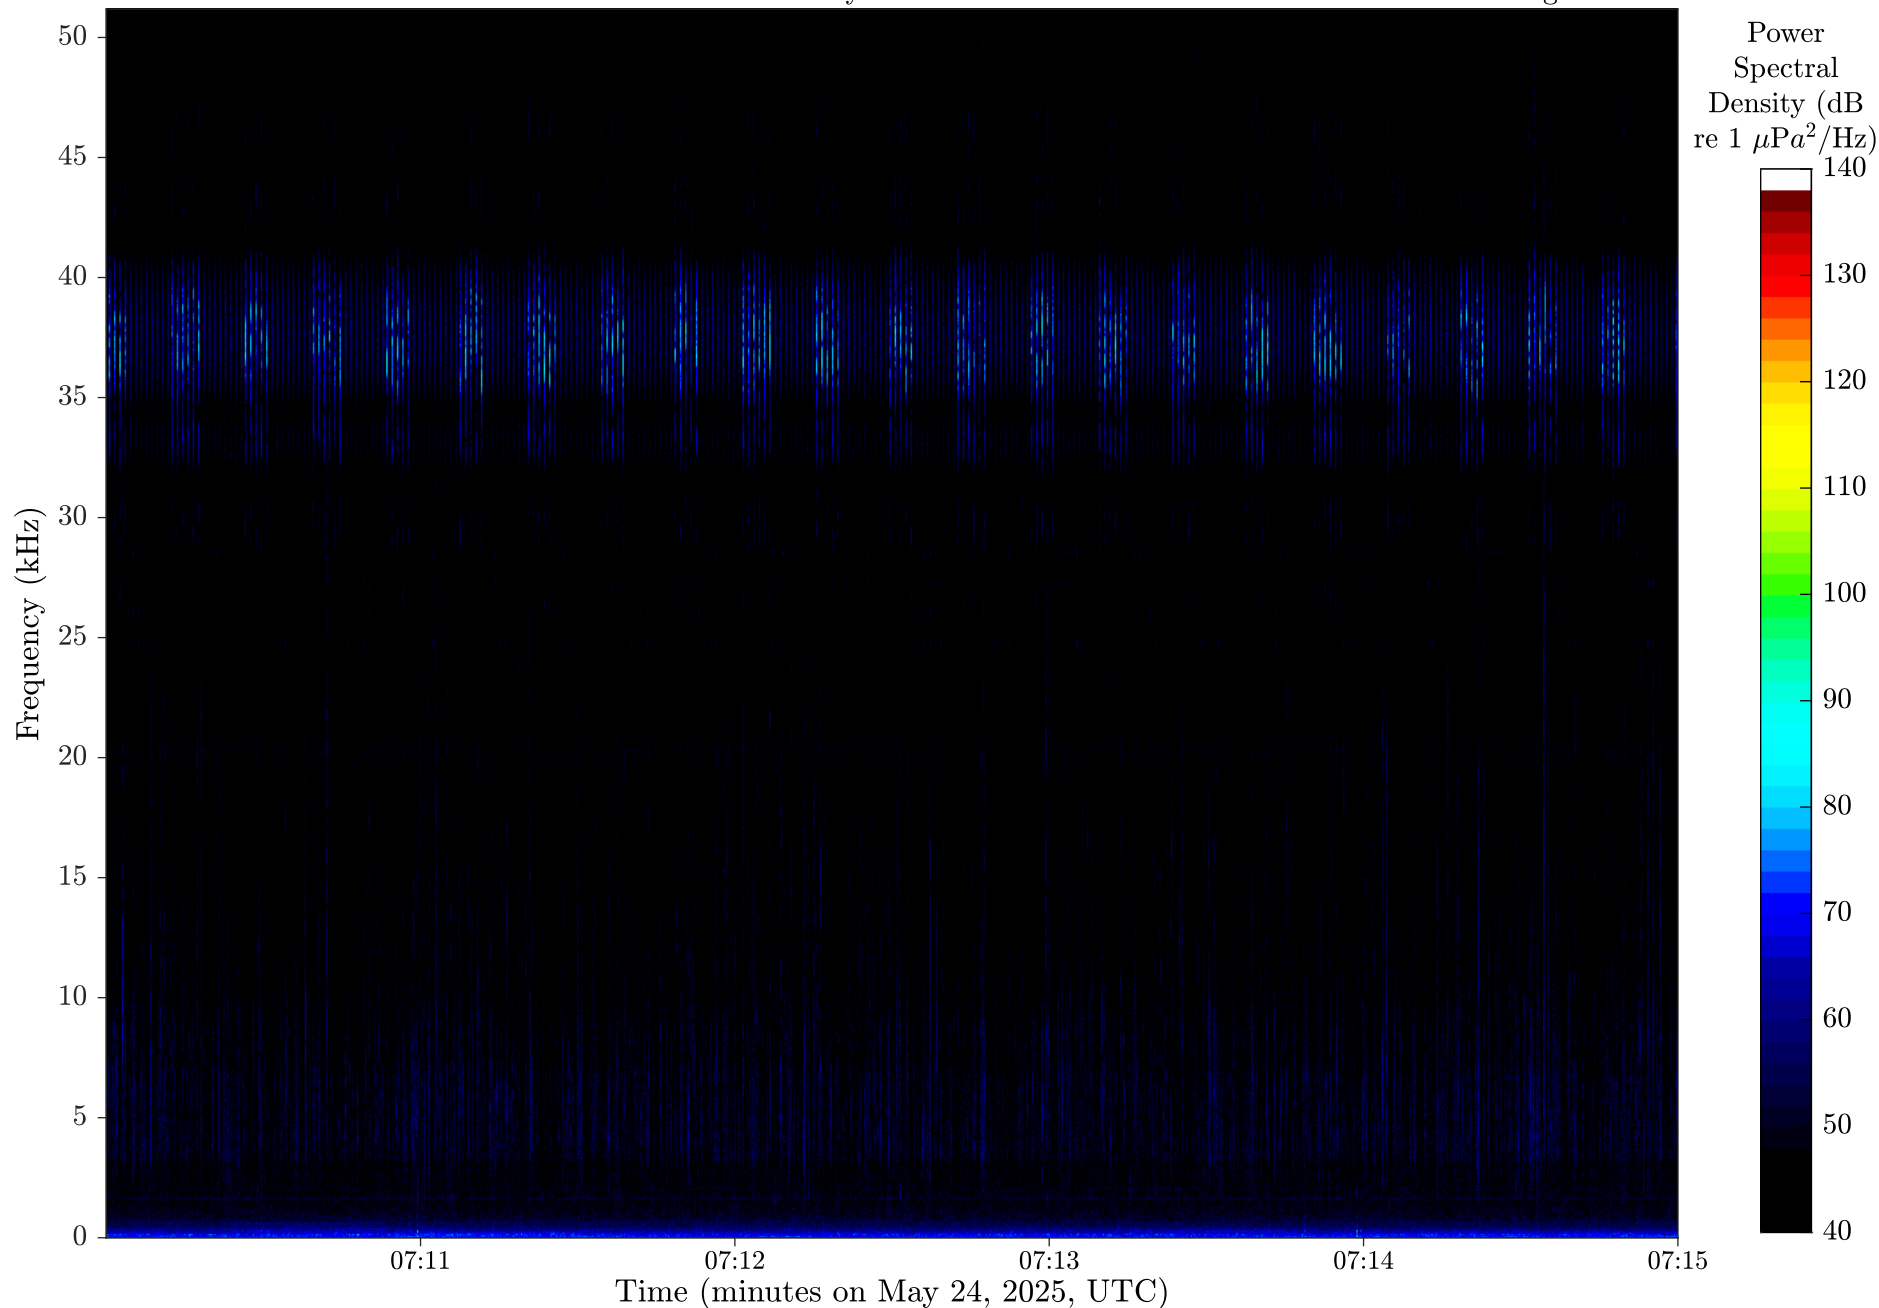


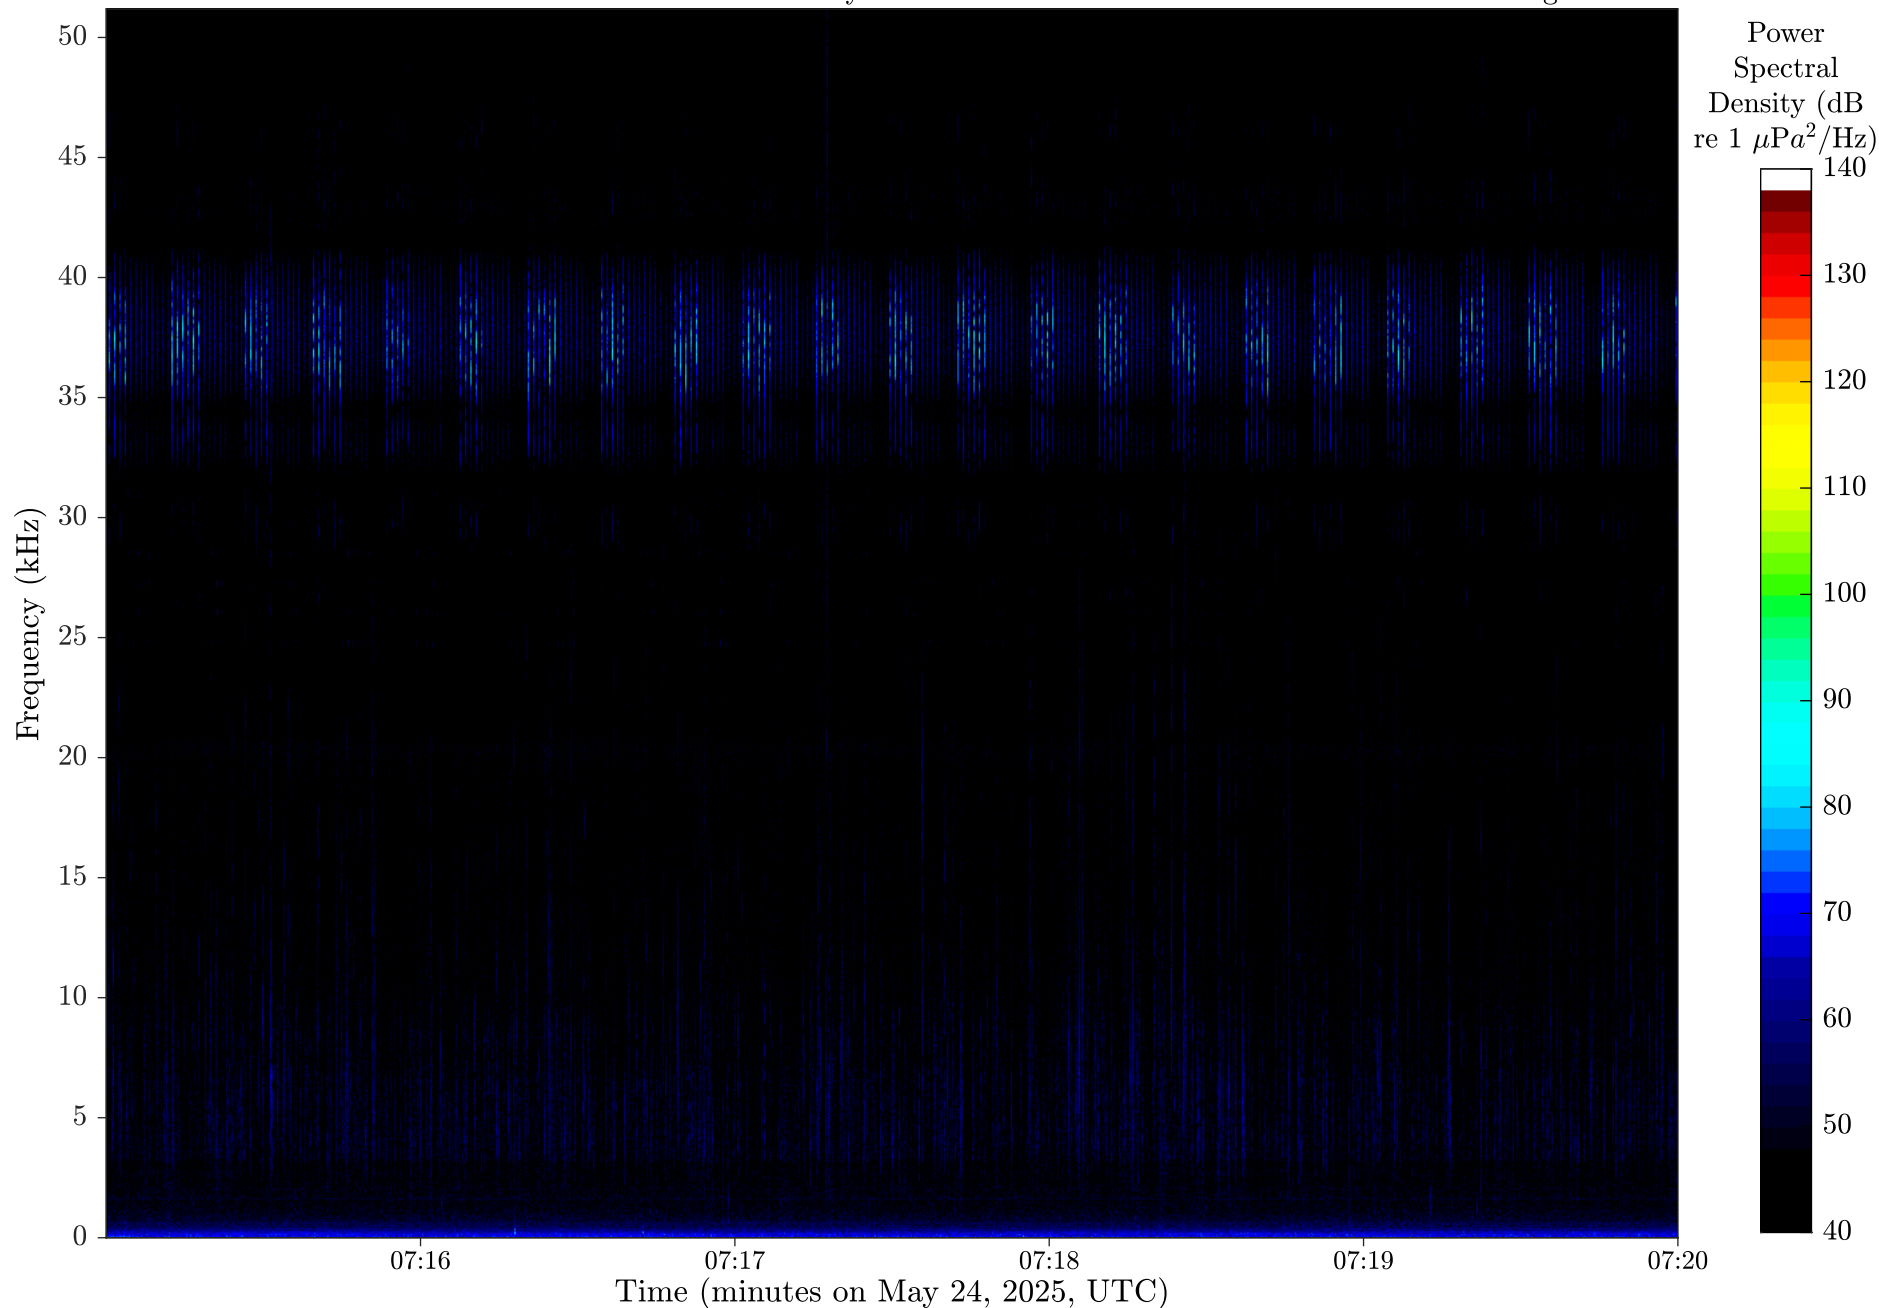


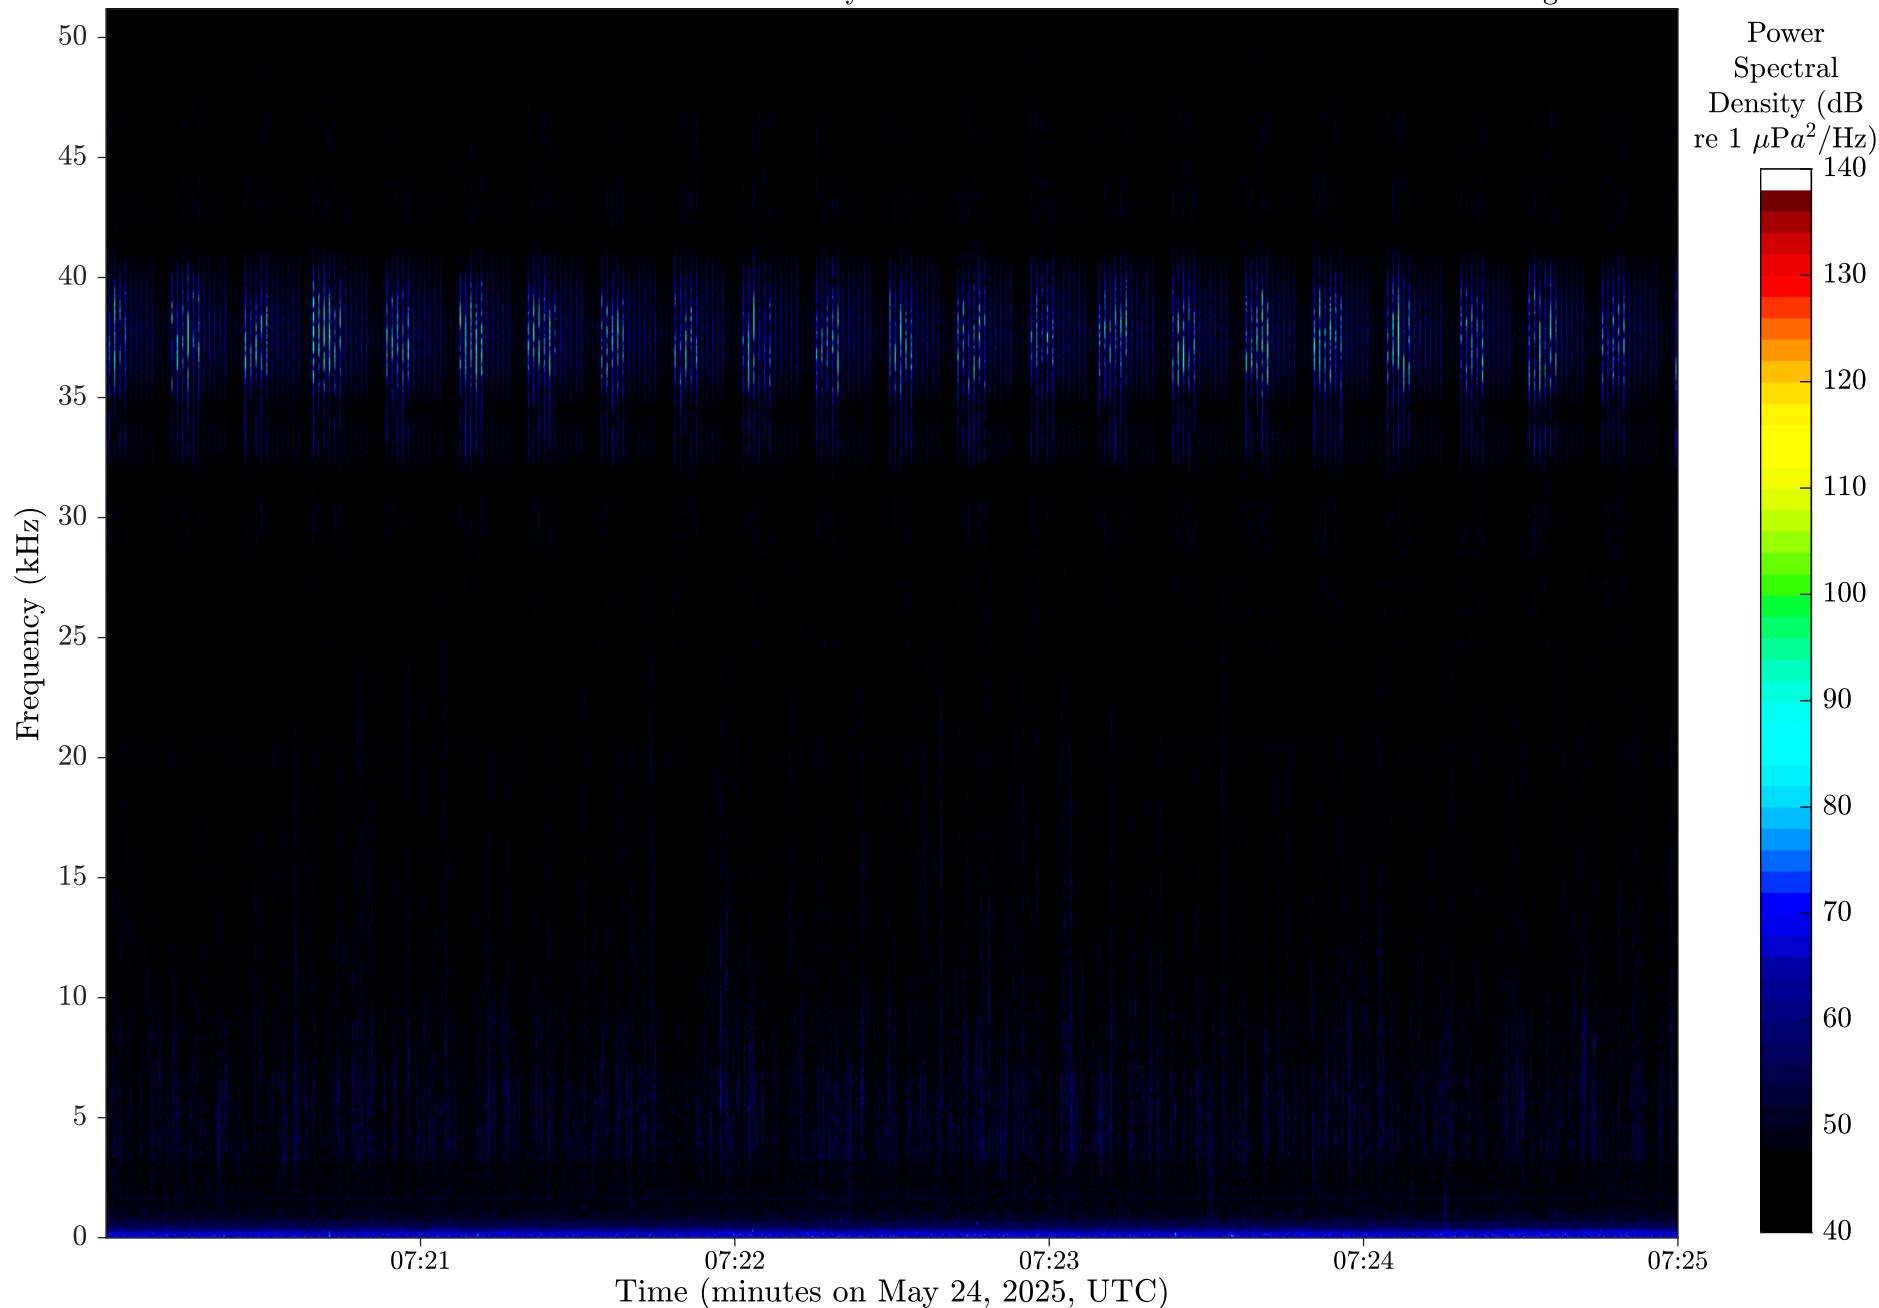

Comments: 36.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:19:23 UTC

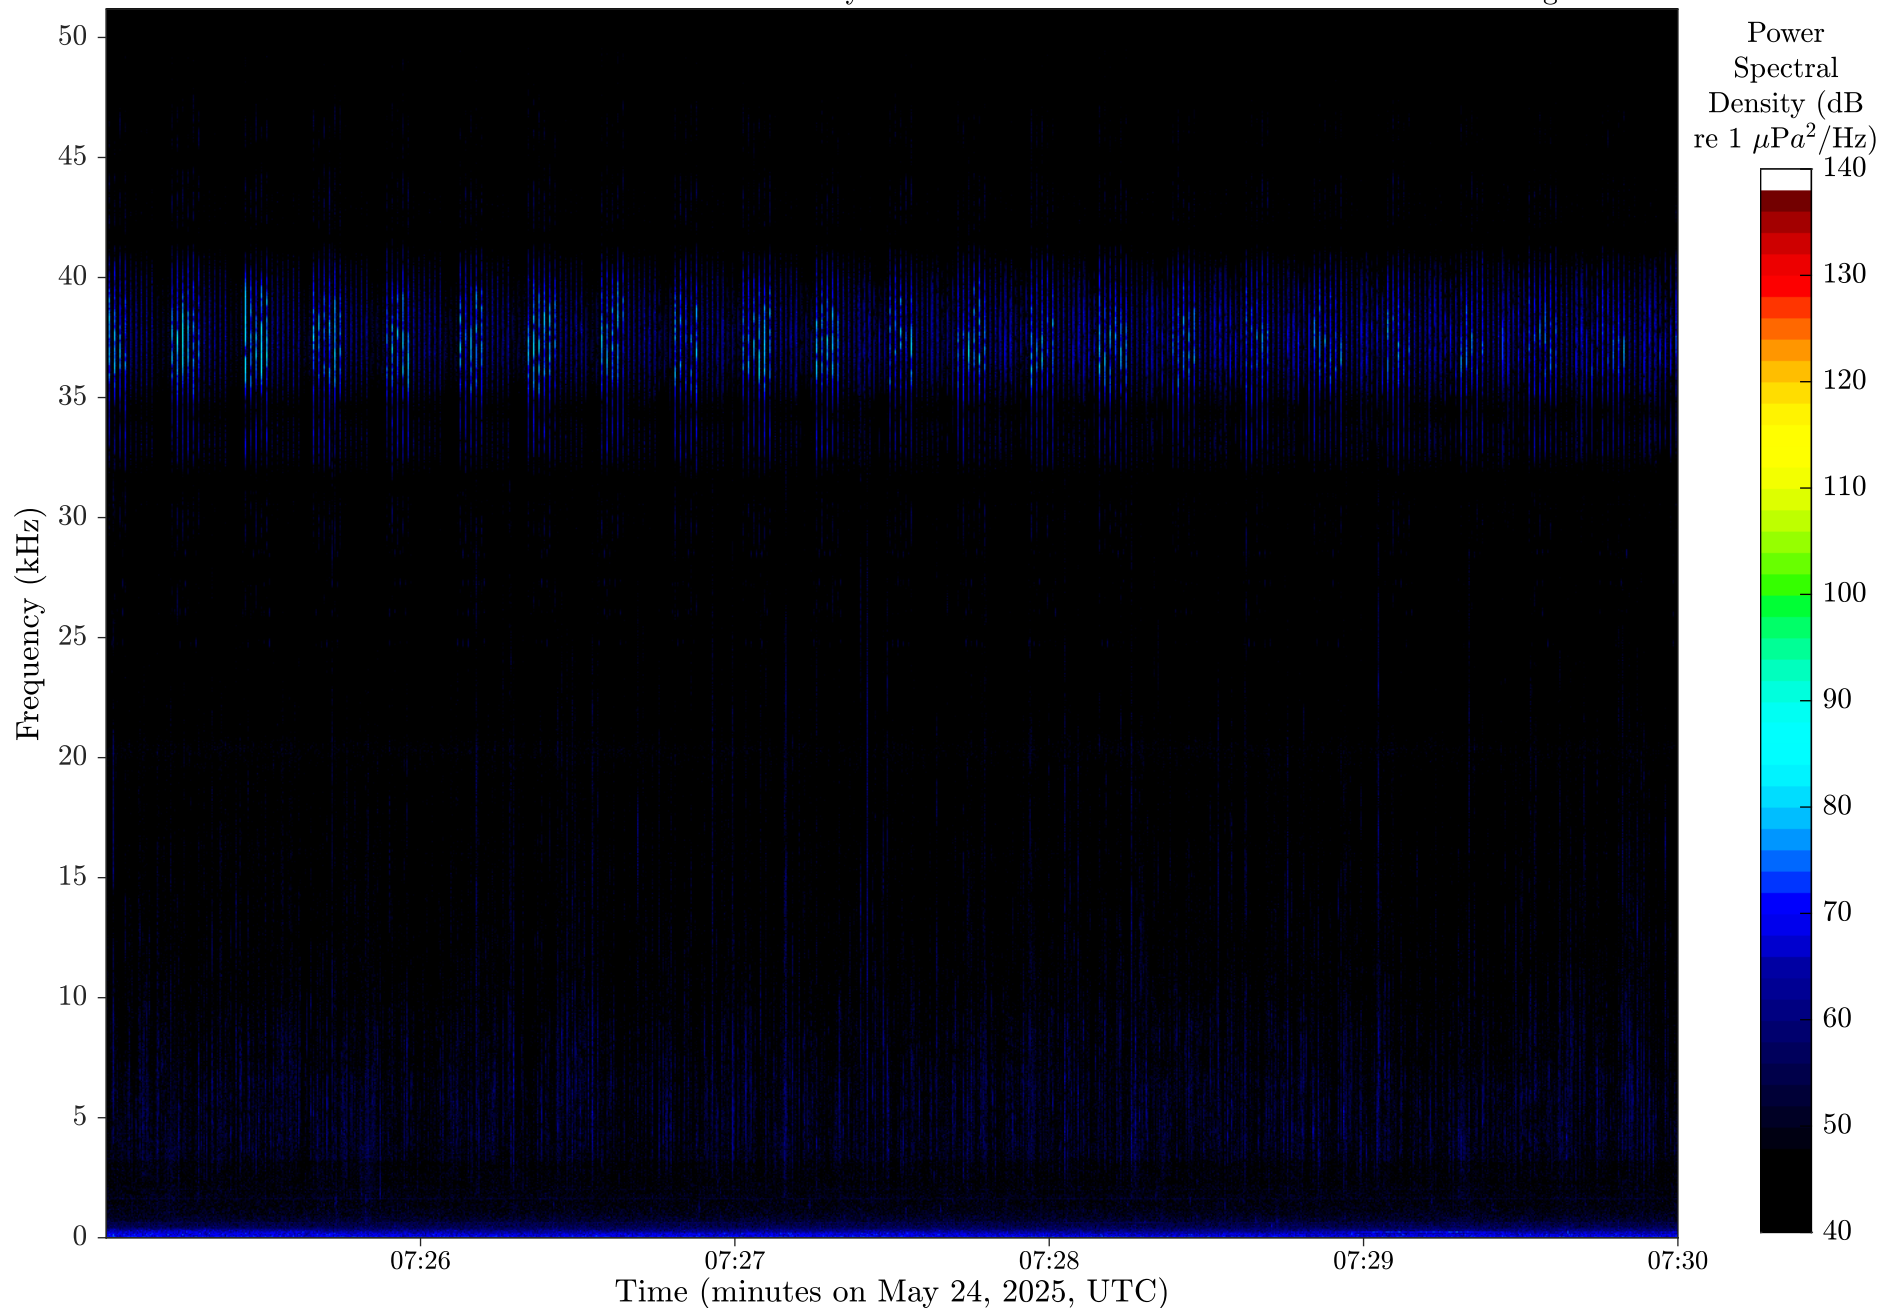

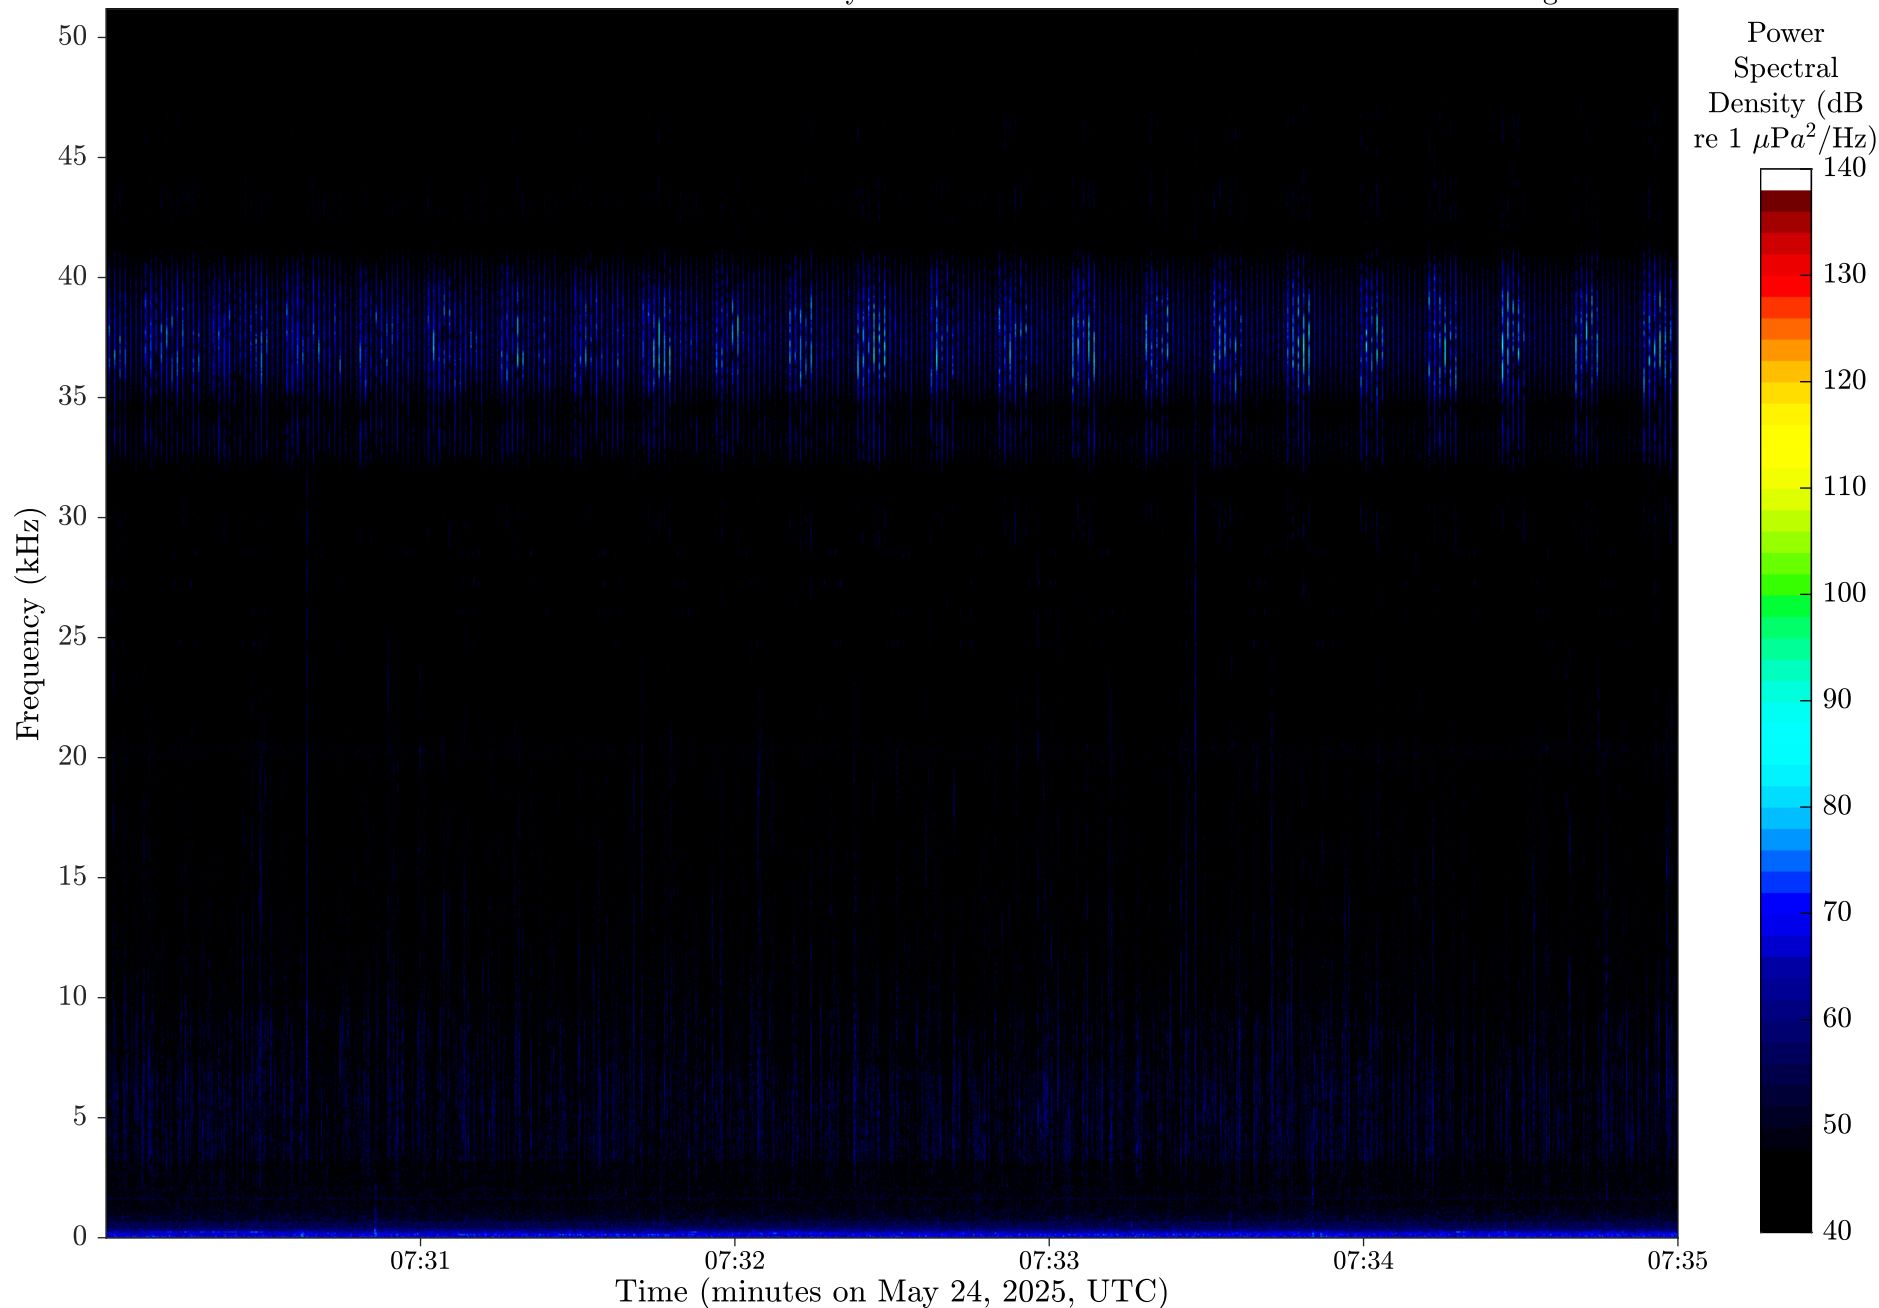


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:19:39 UTC

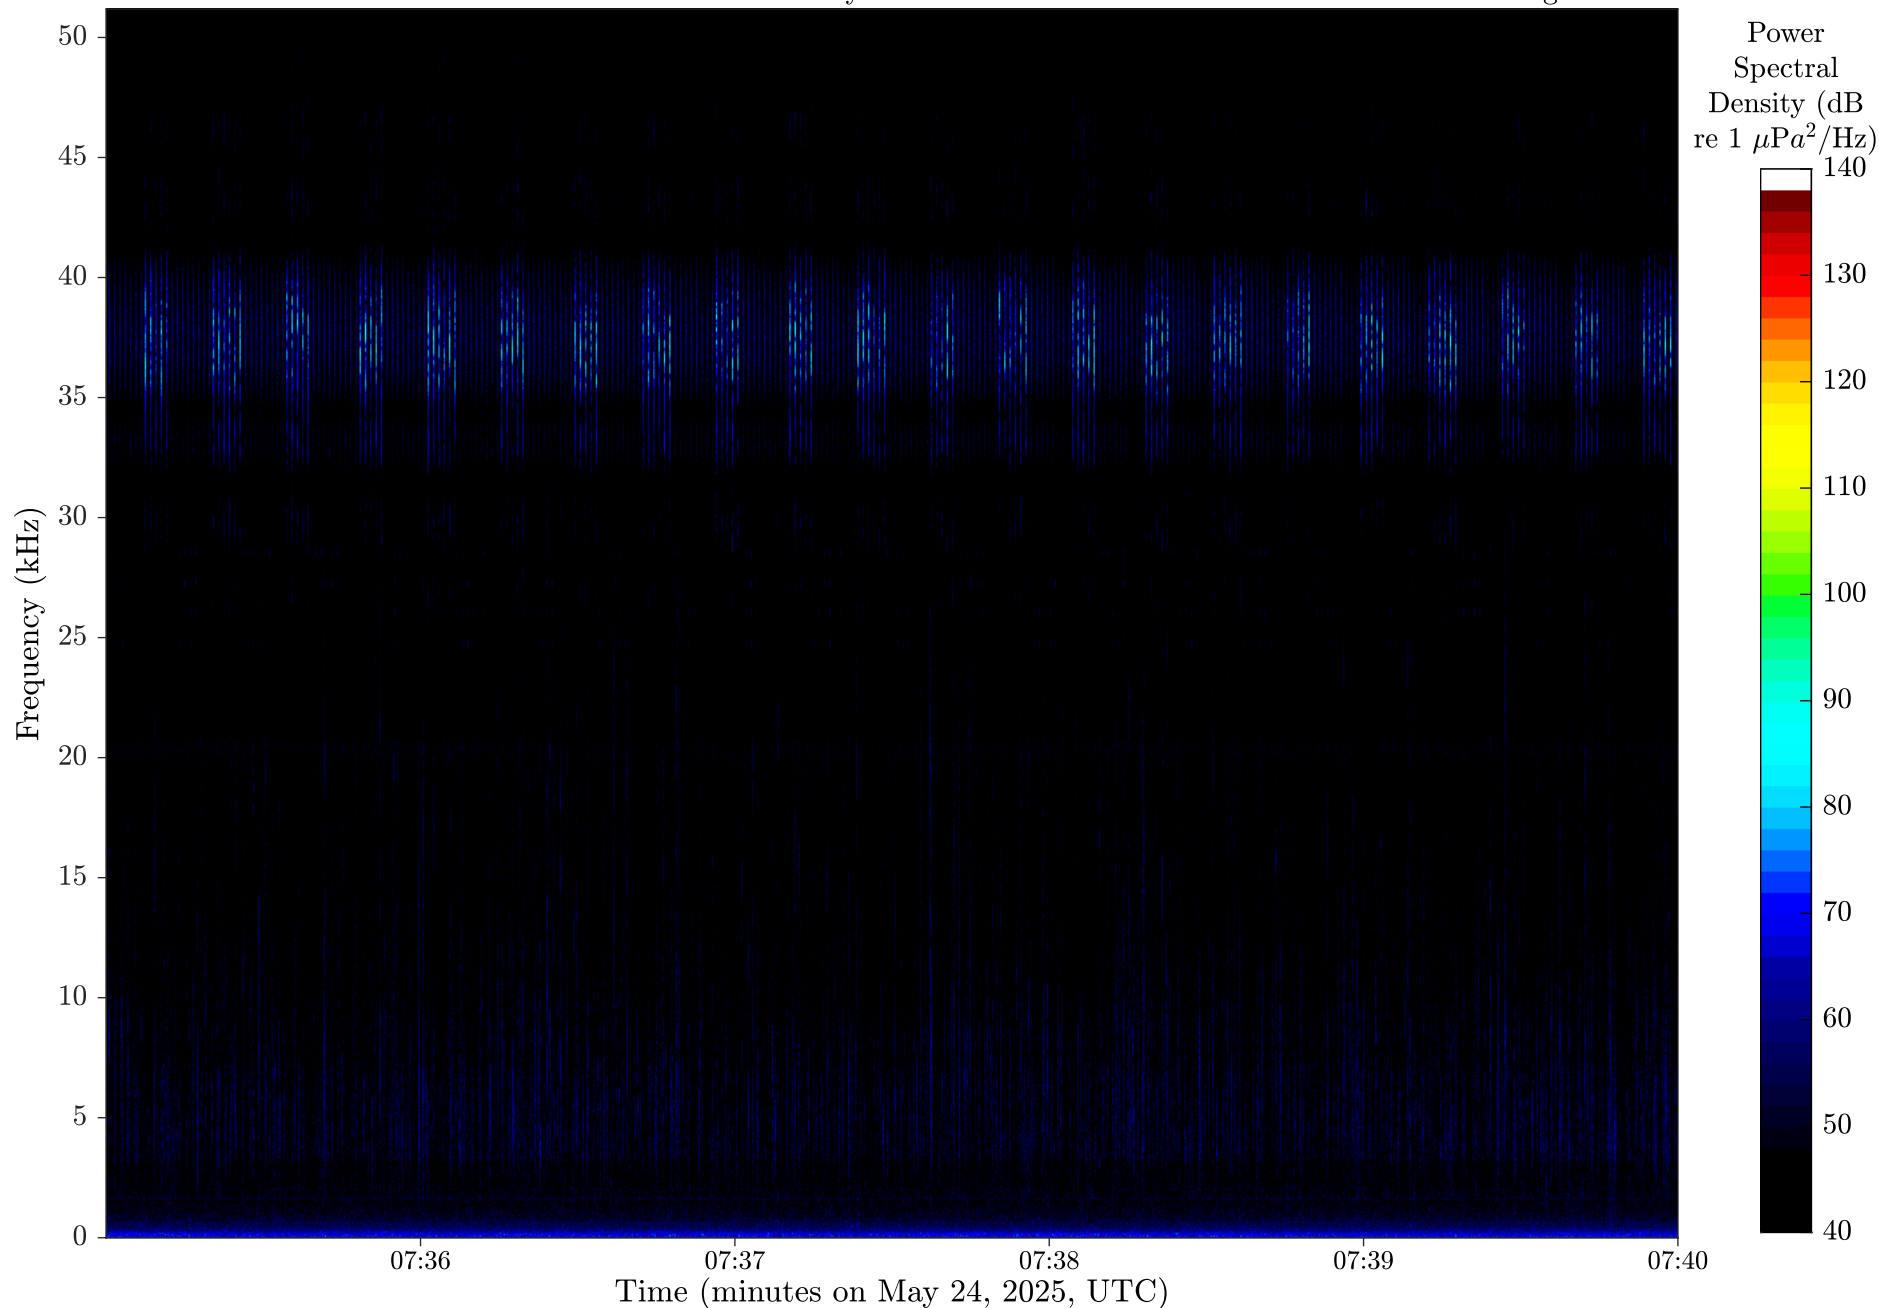


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:19:47 UTC

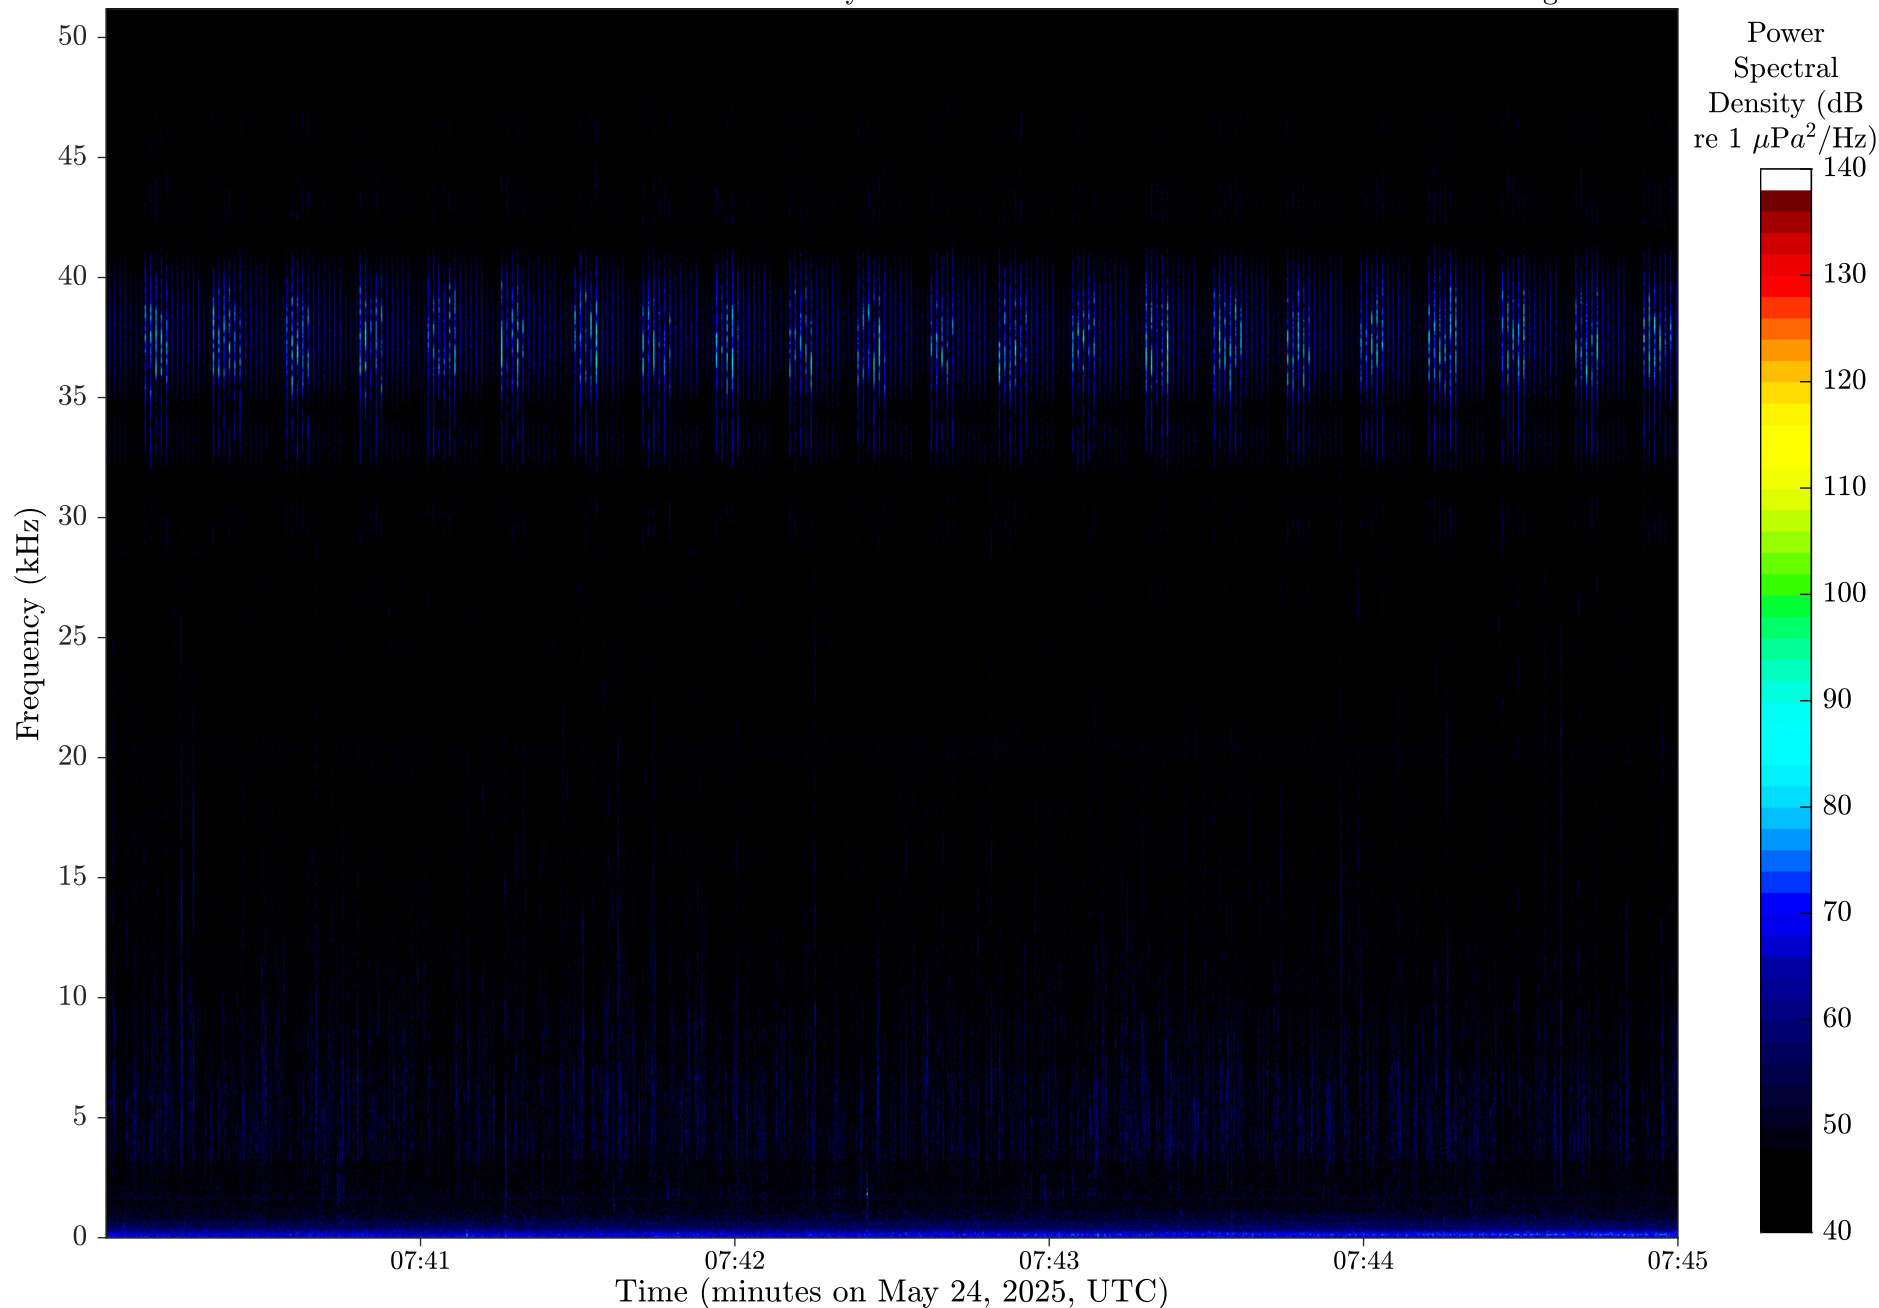


Comments: 36.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:19:56 UTC

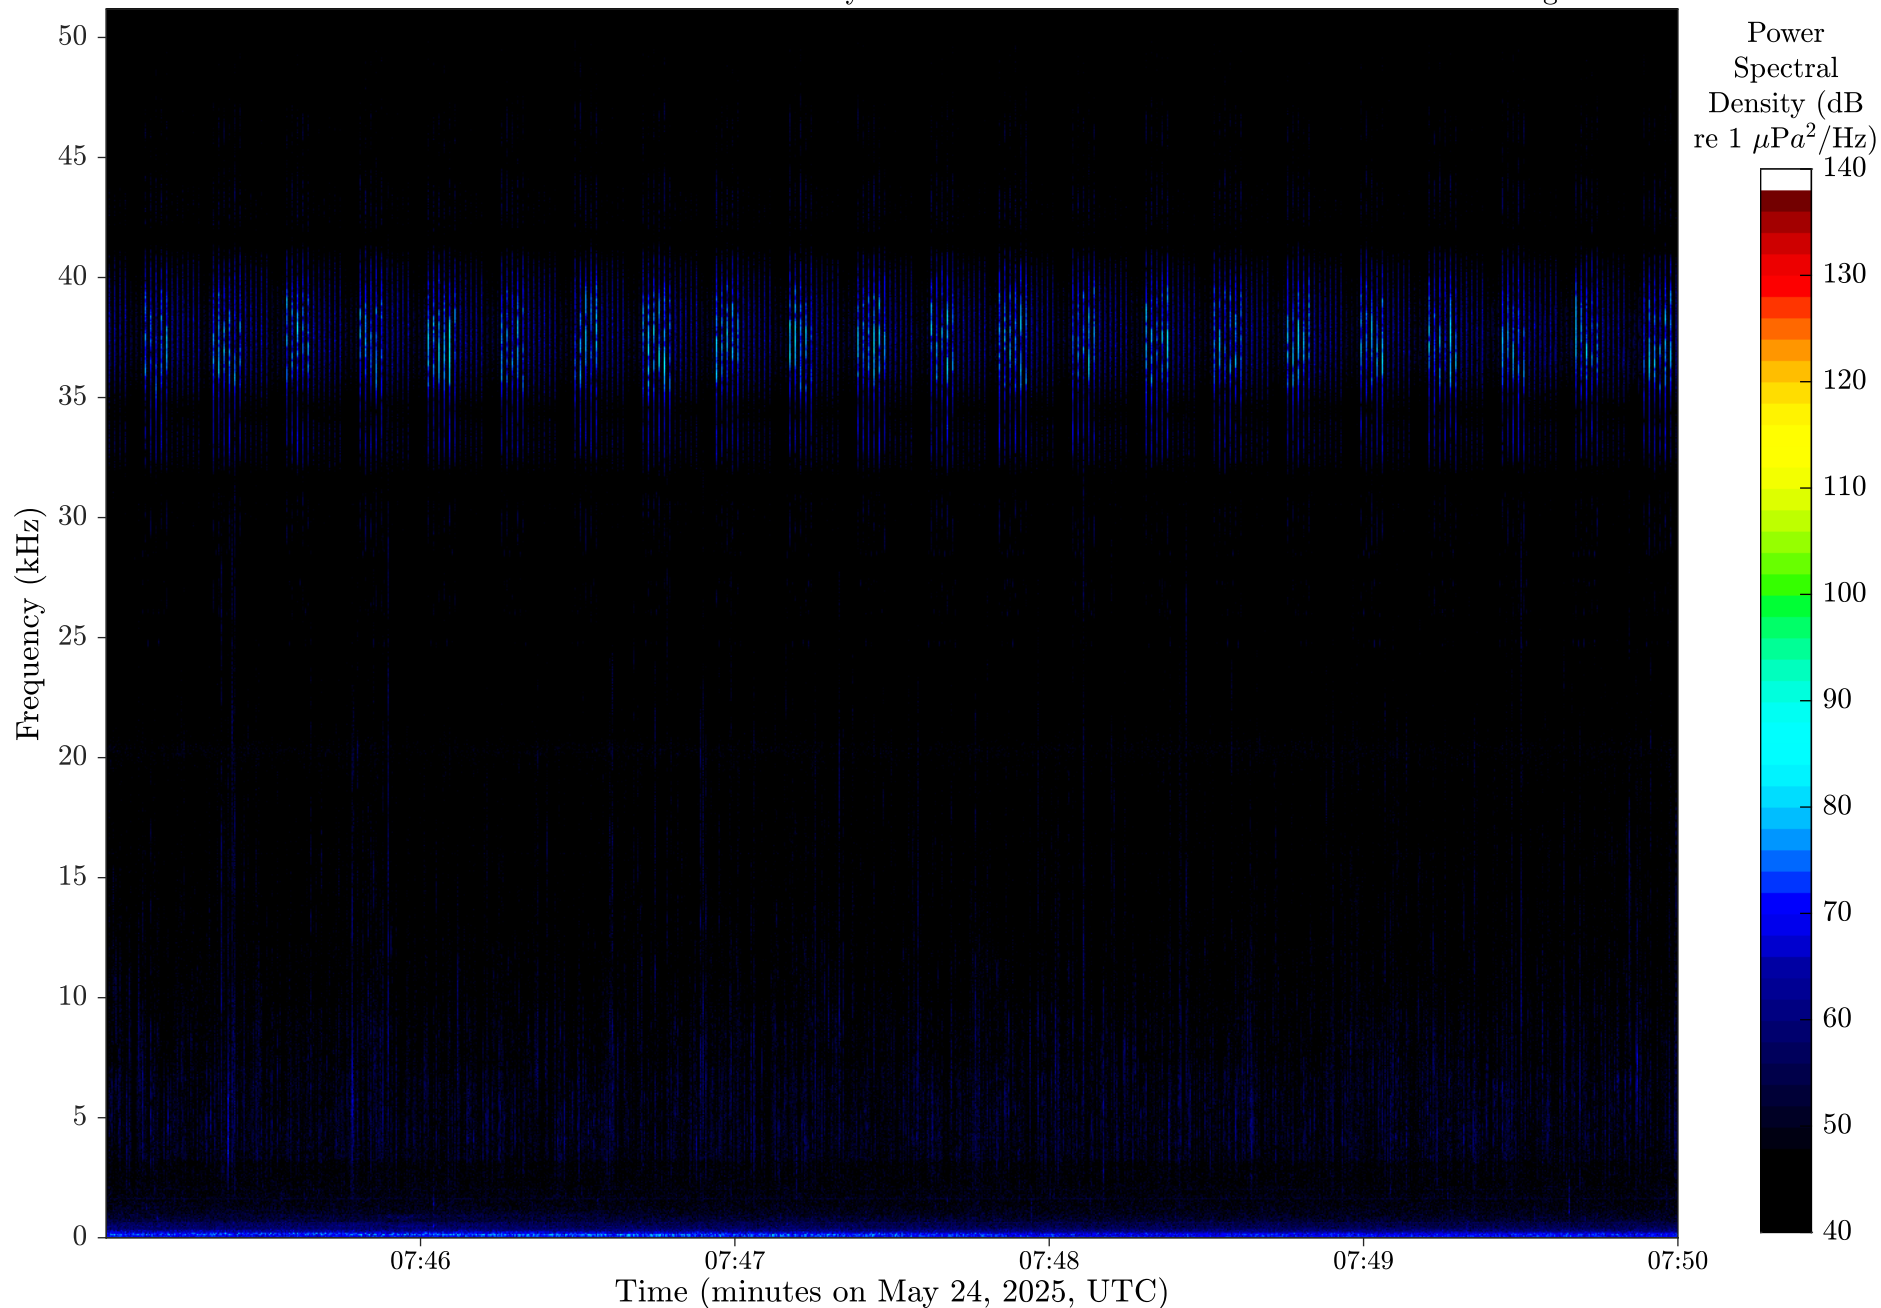


Comments: 36.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:20:03 UTC

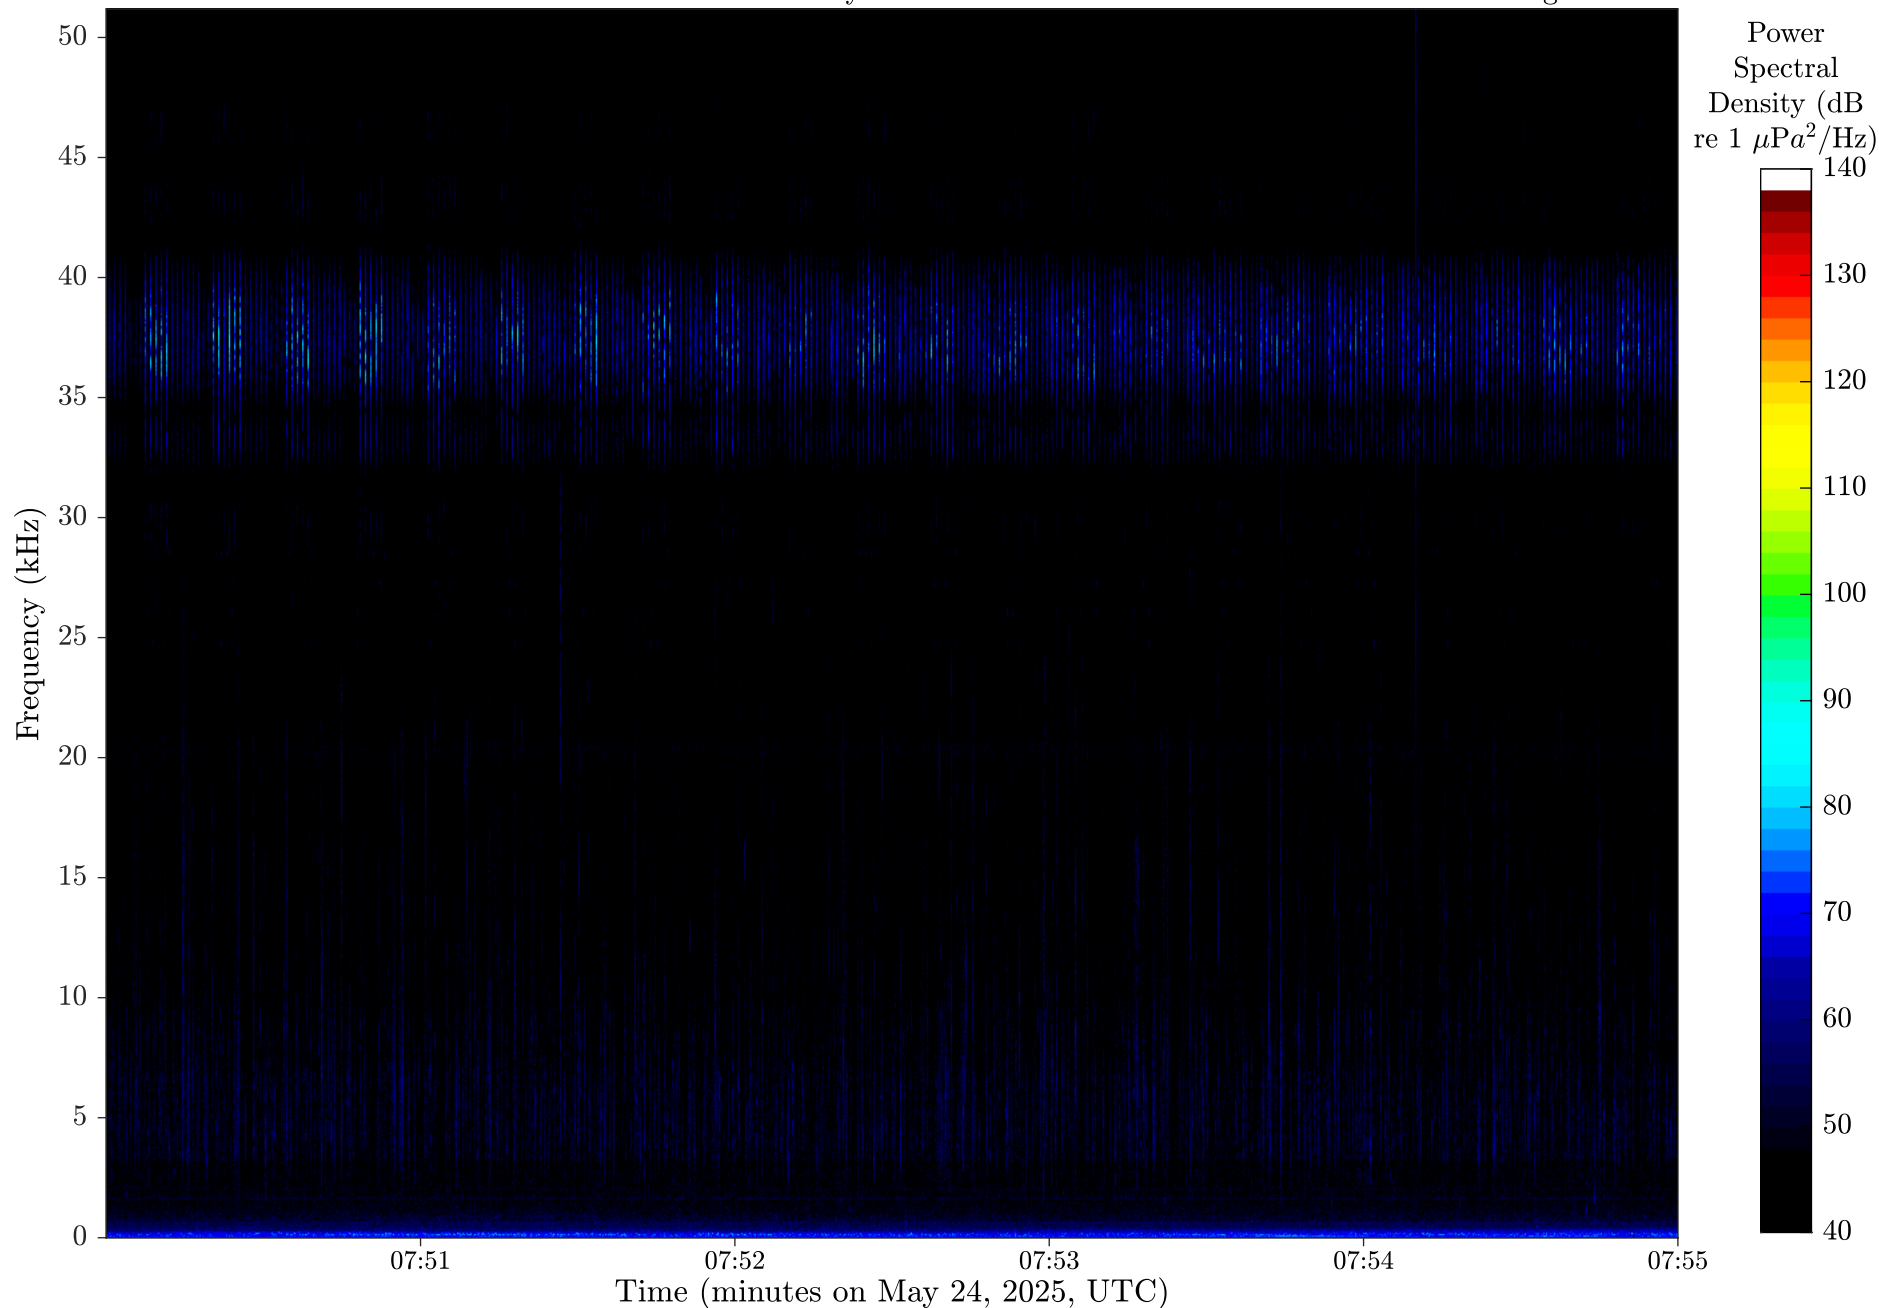

Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:20:11 UTC

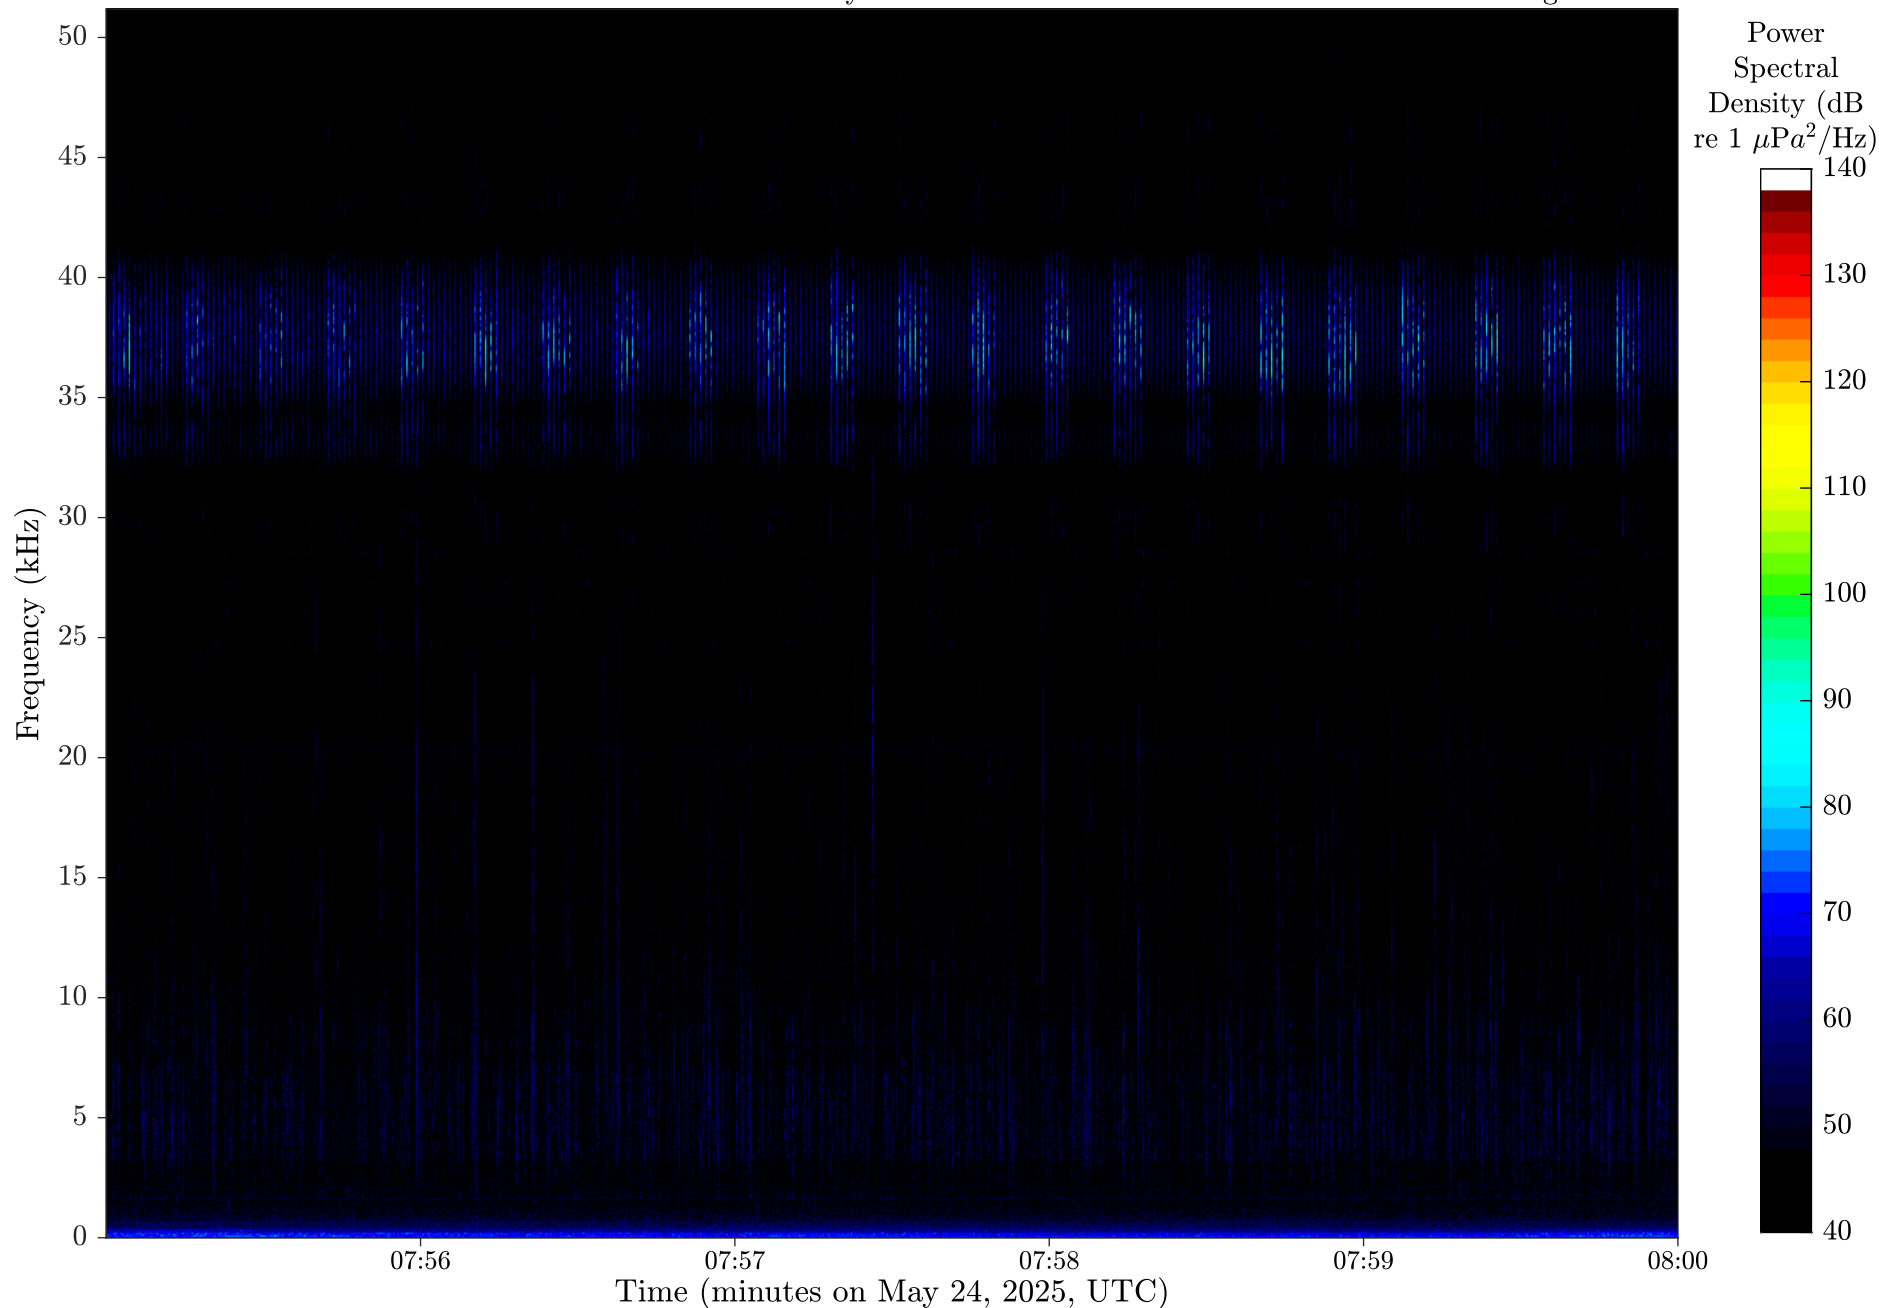

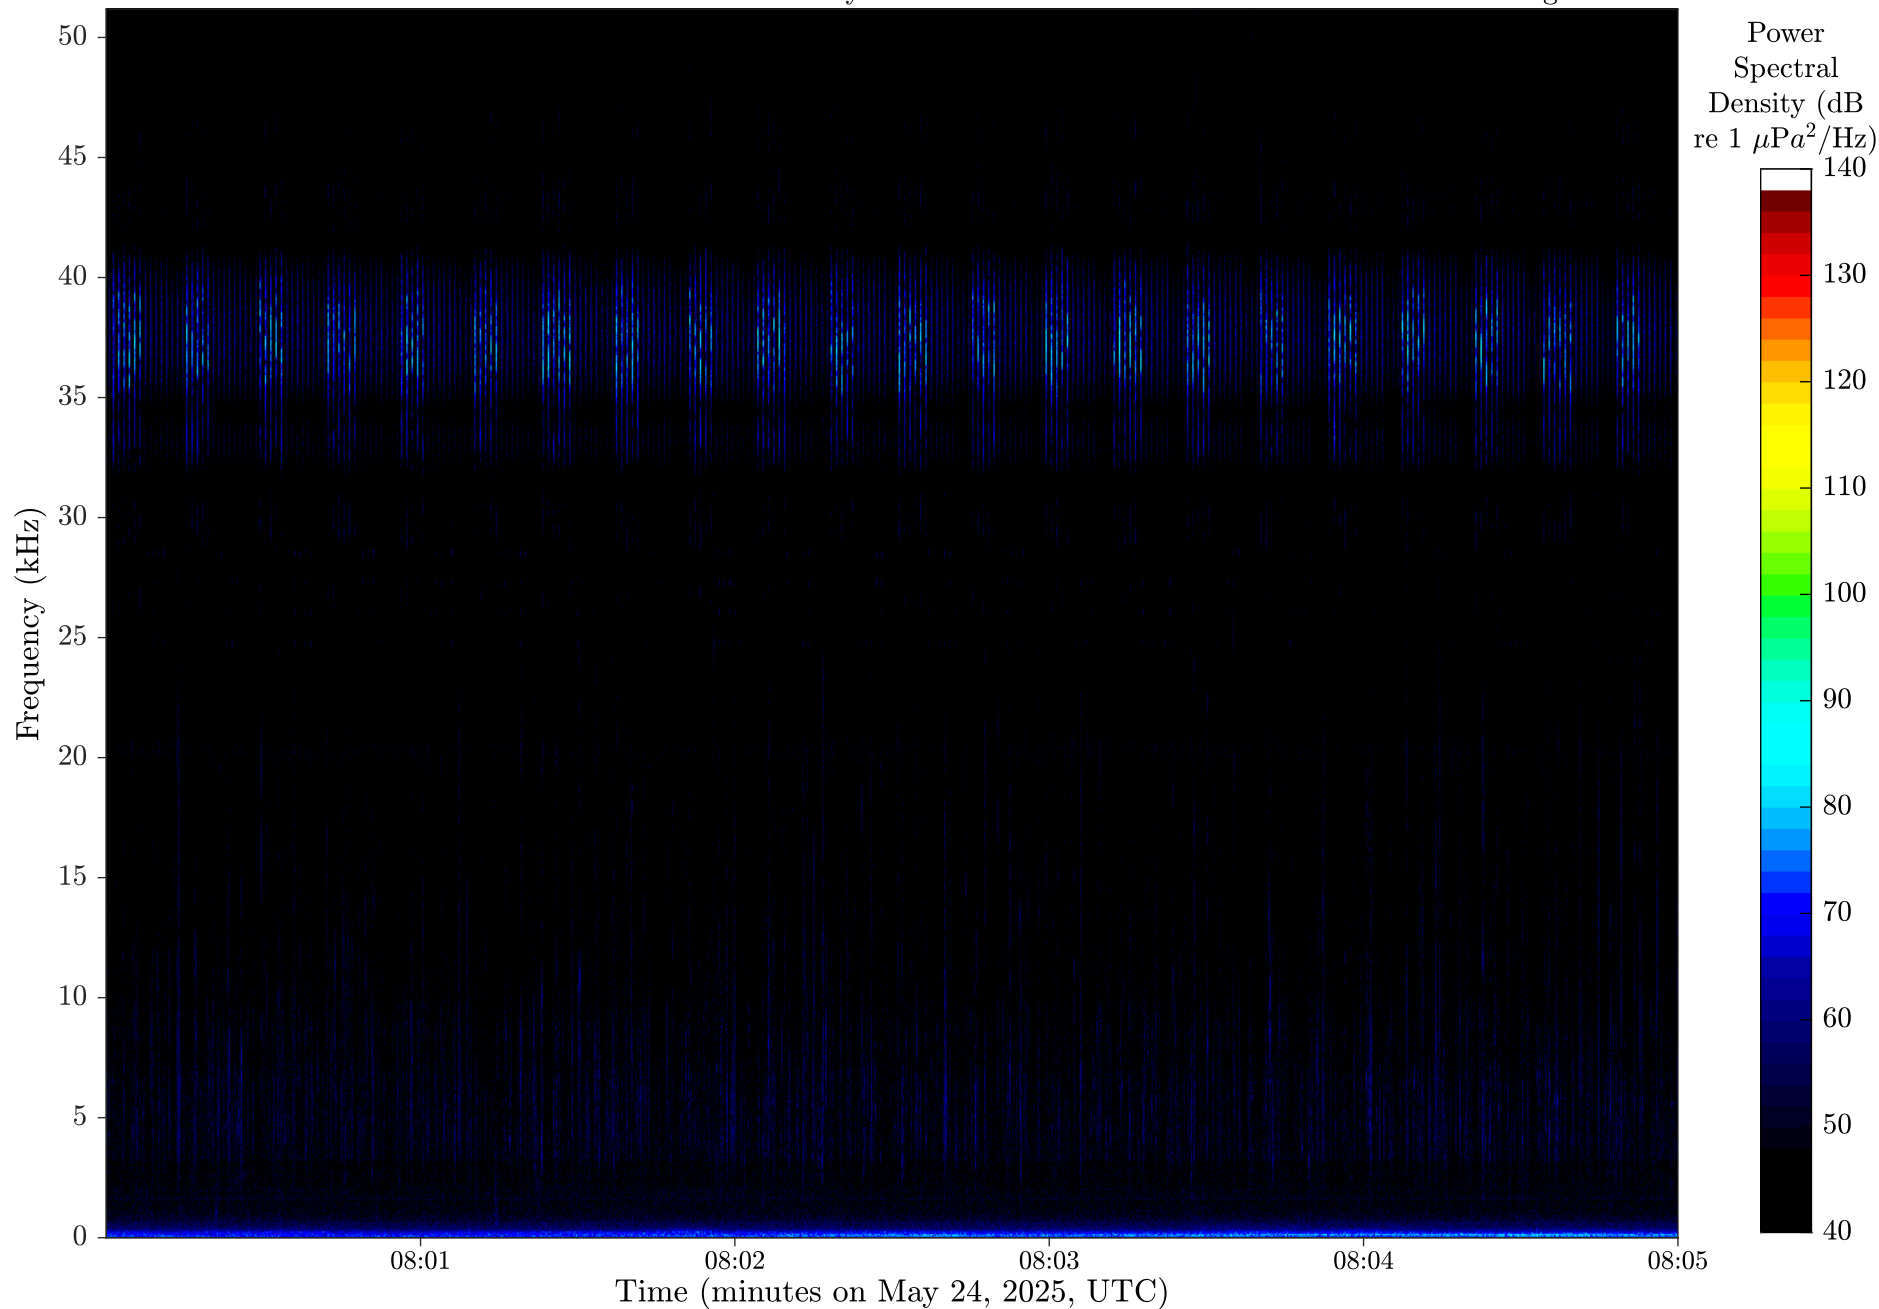


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:27 UTC

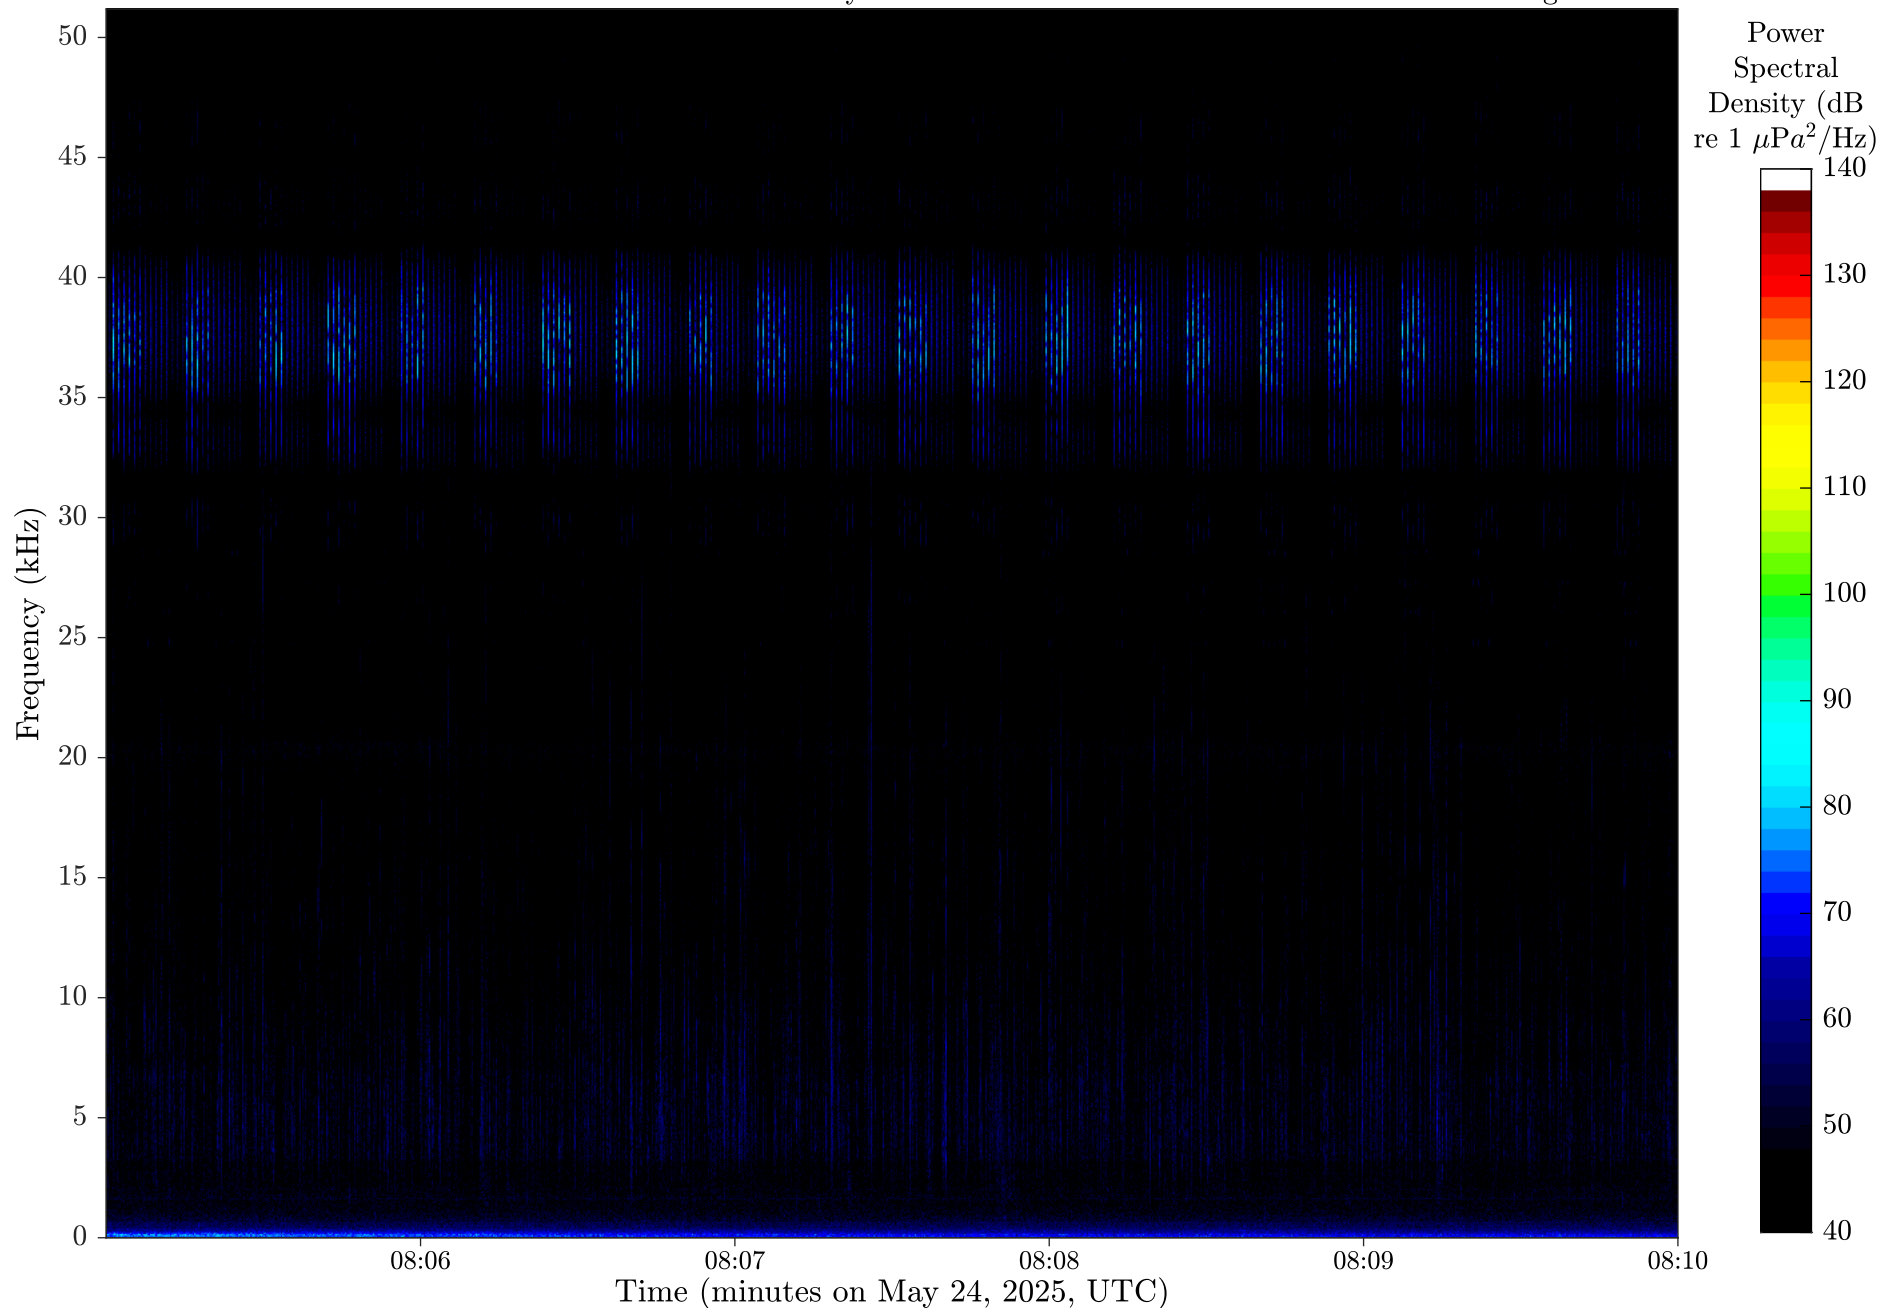


Comments: 36.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:35 UTC

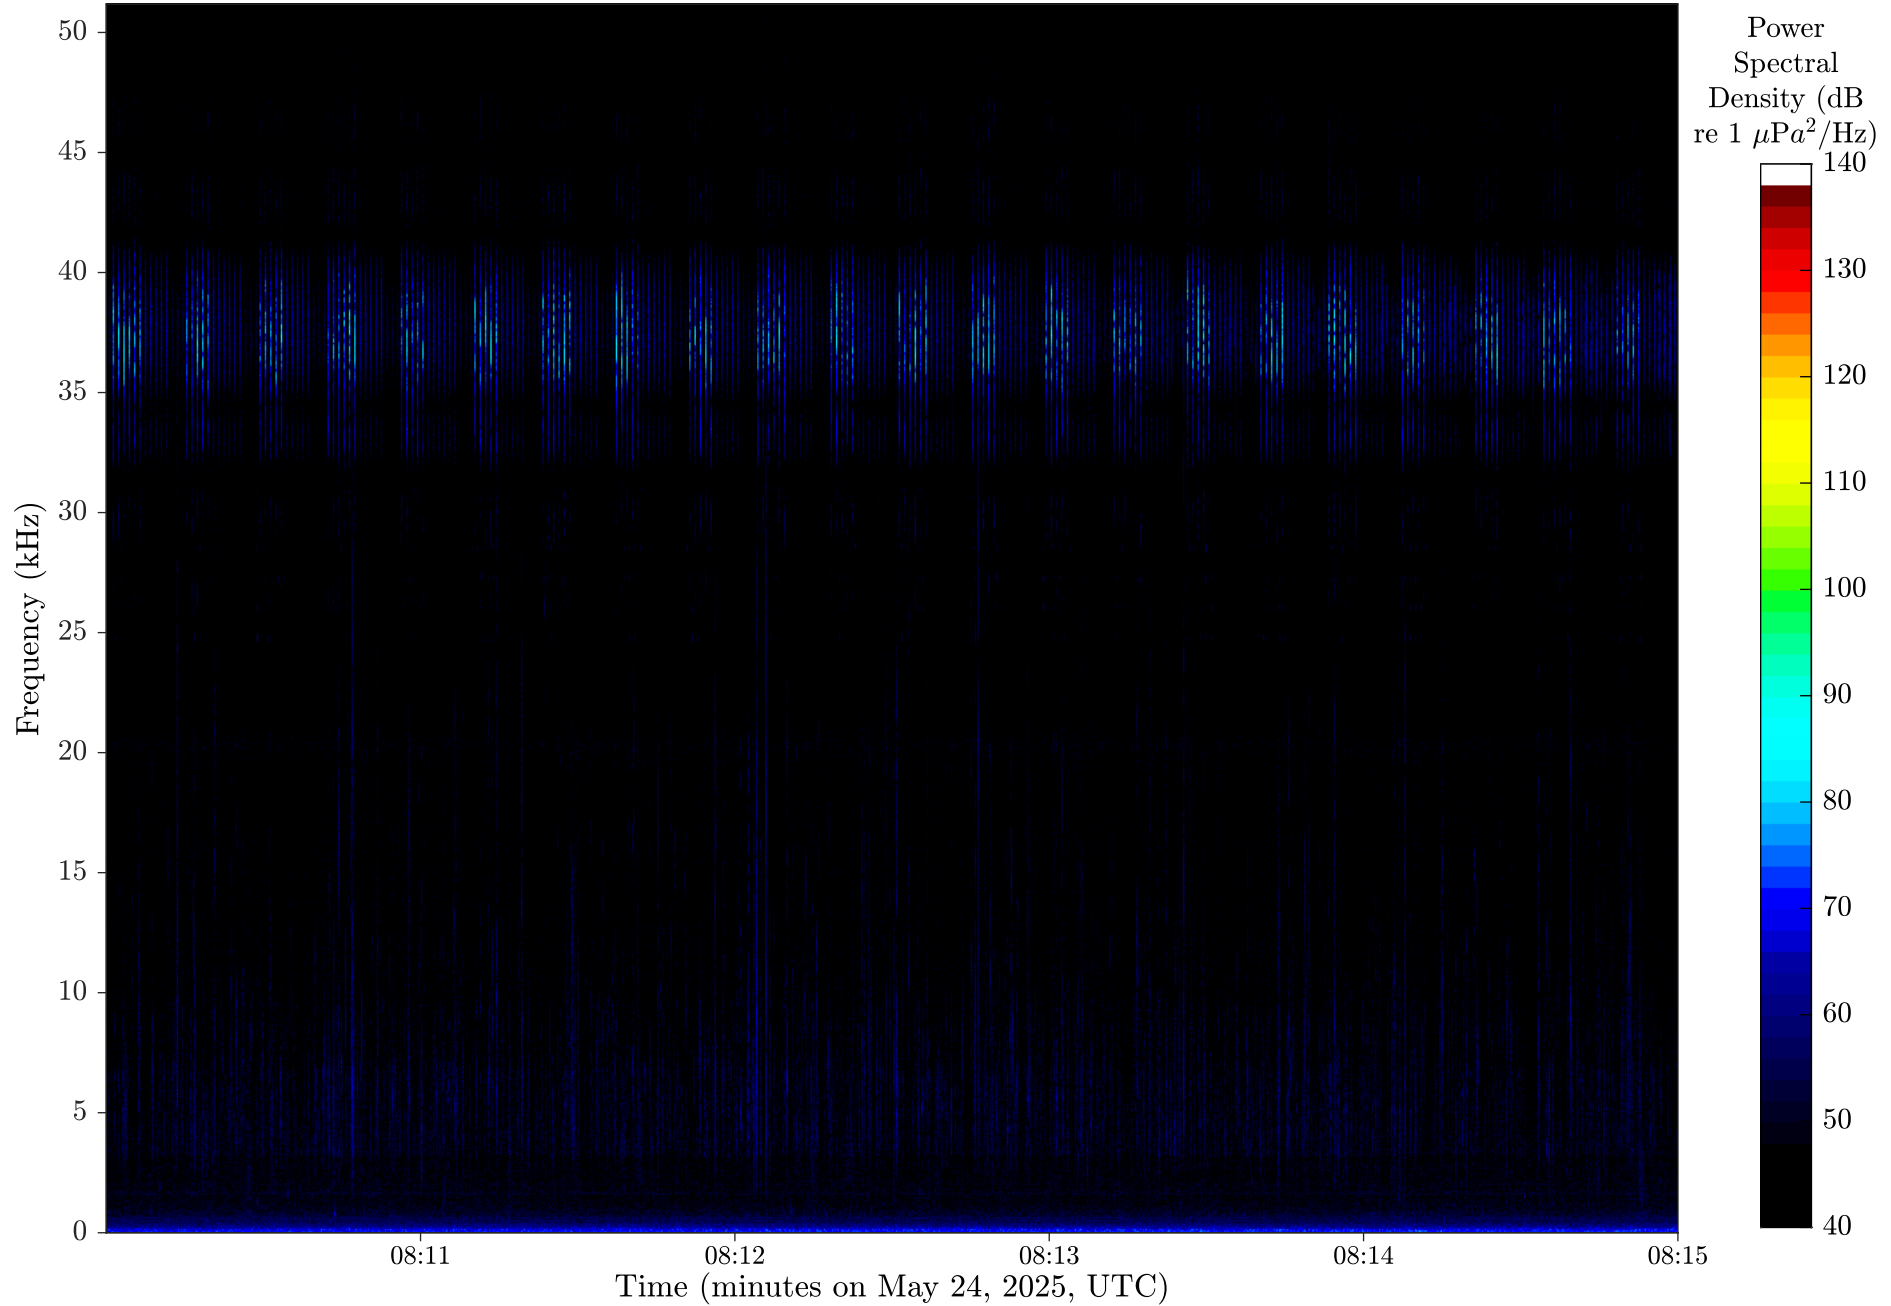


Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:43 UTC

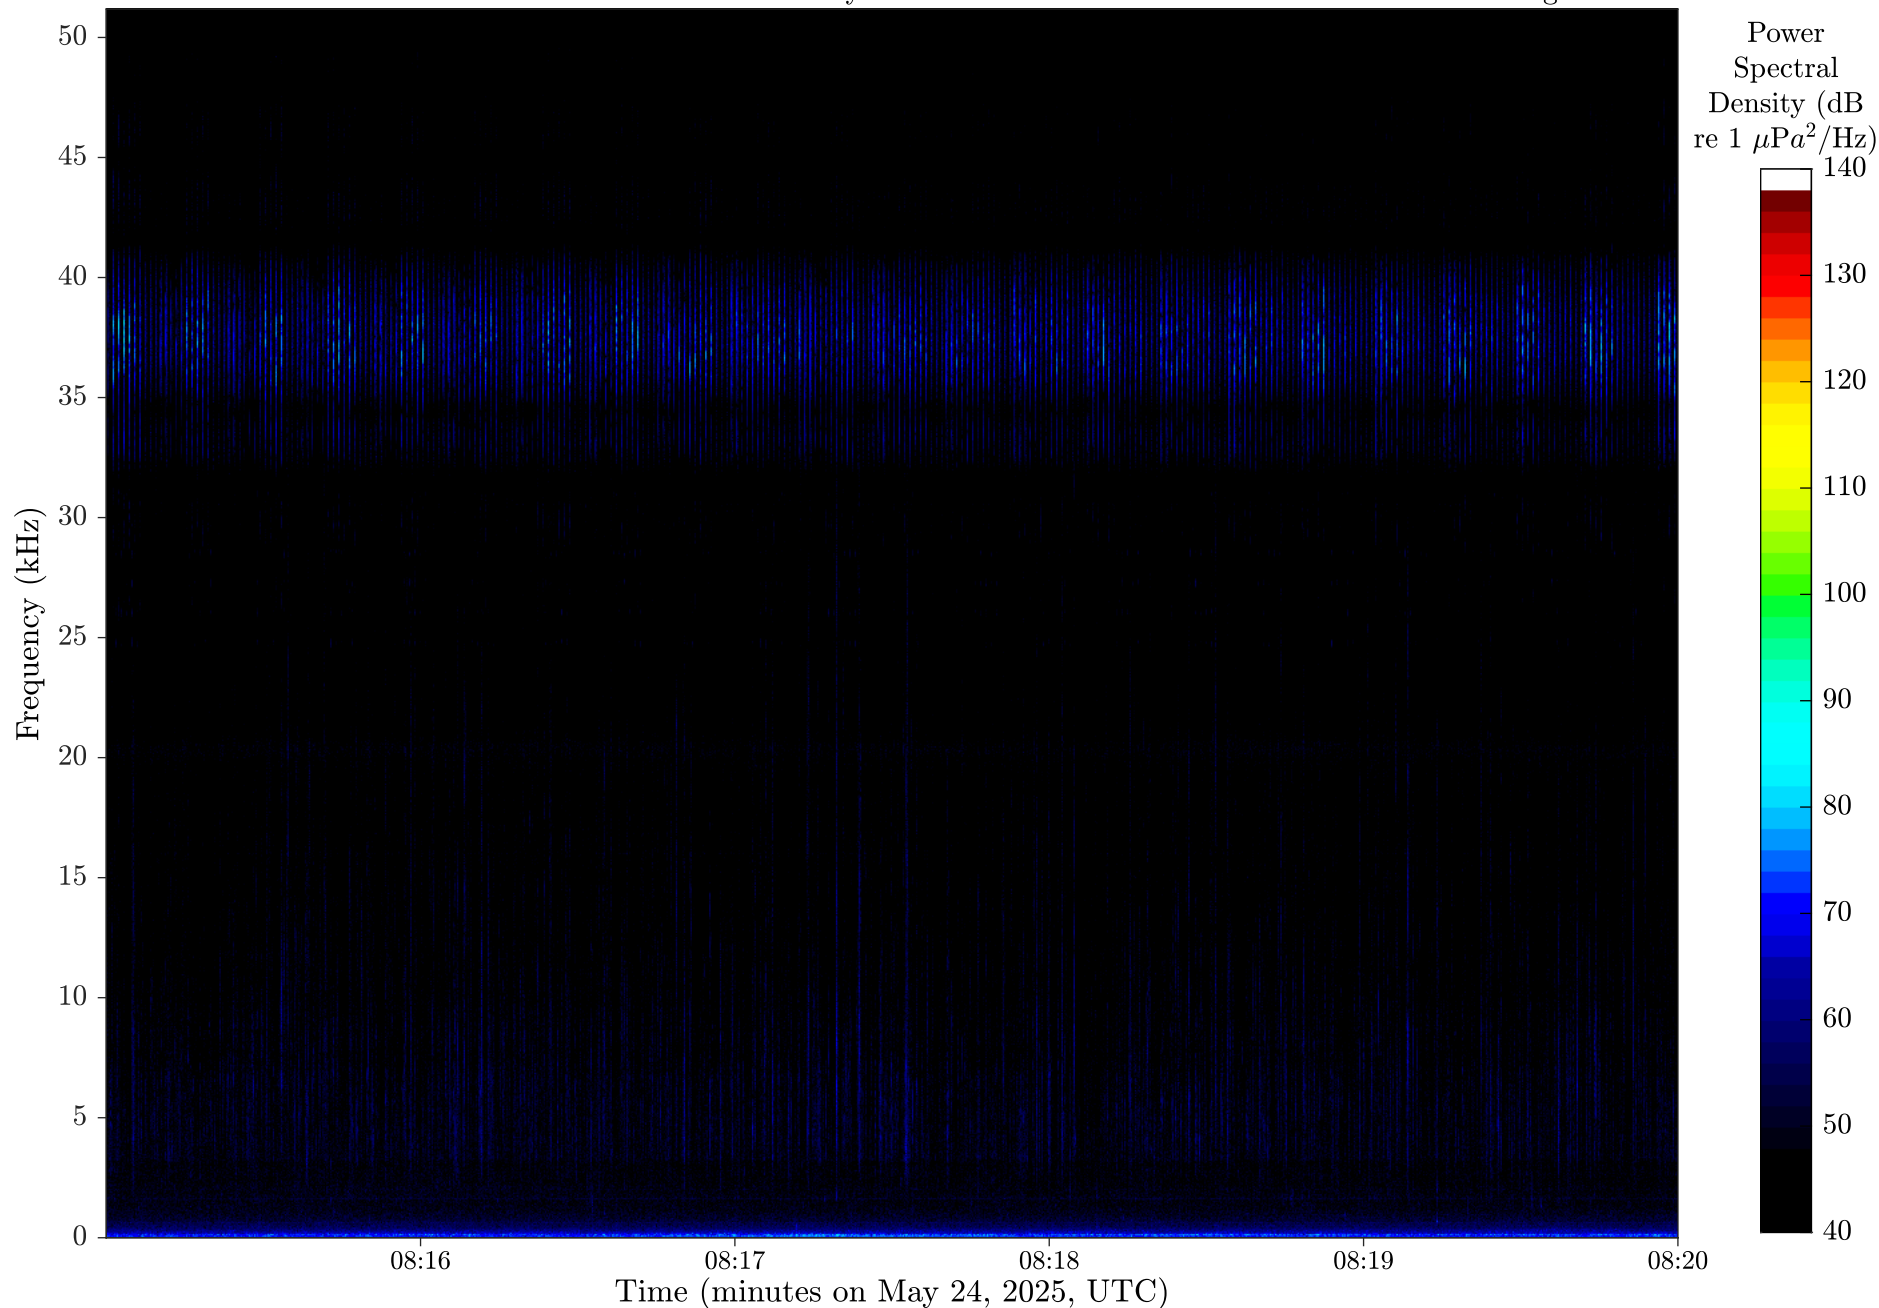


Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:50 UTC

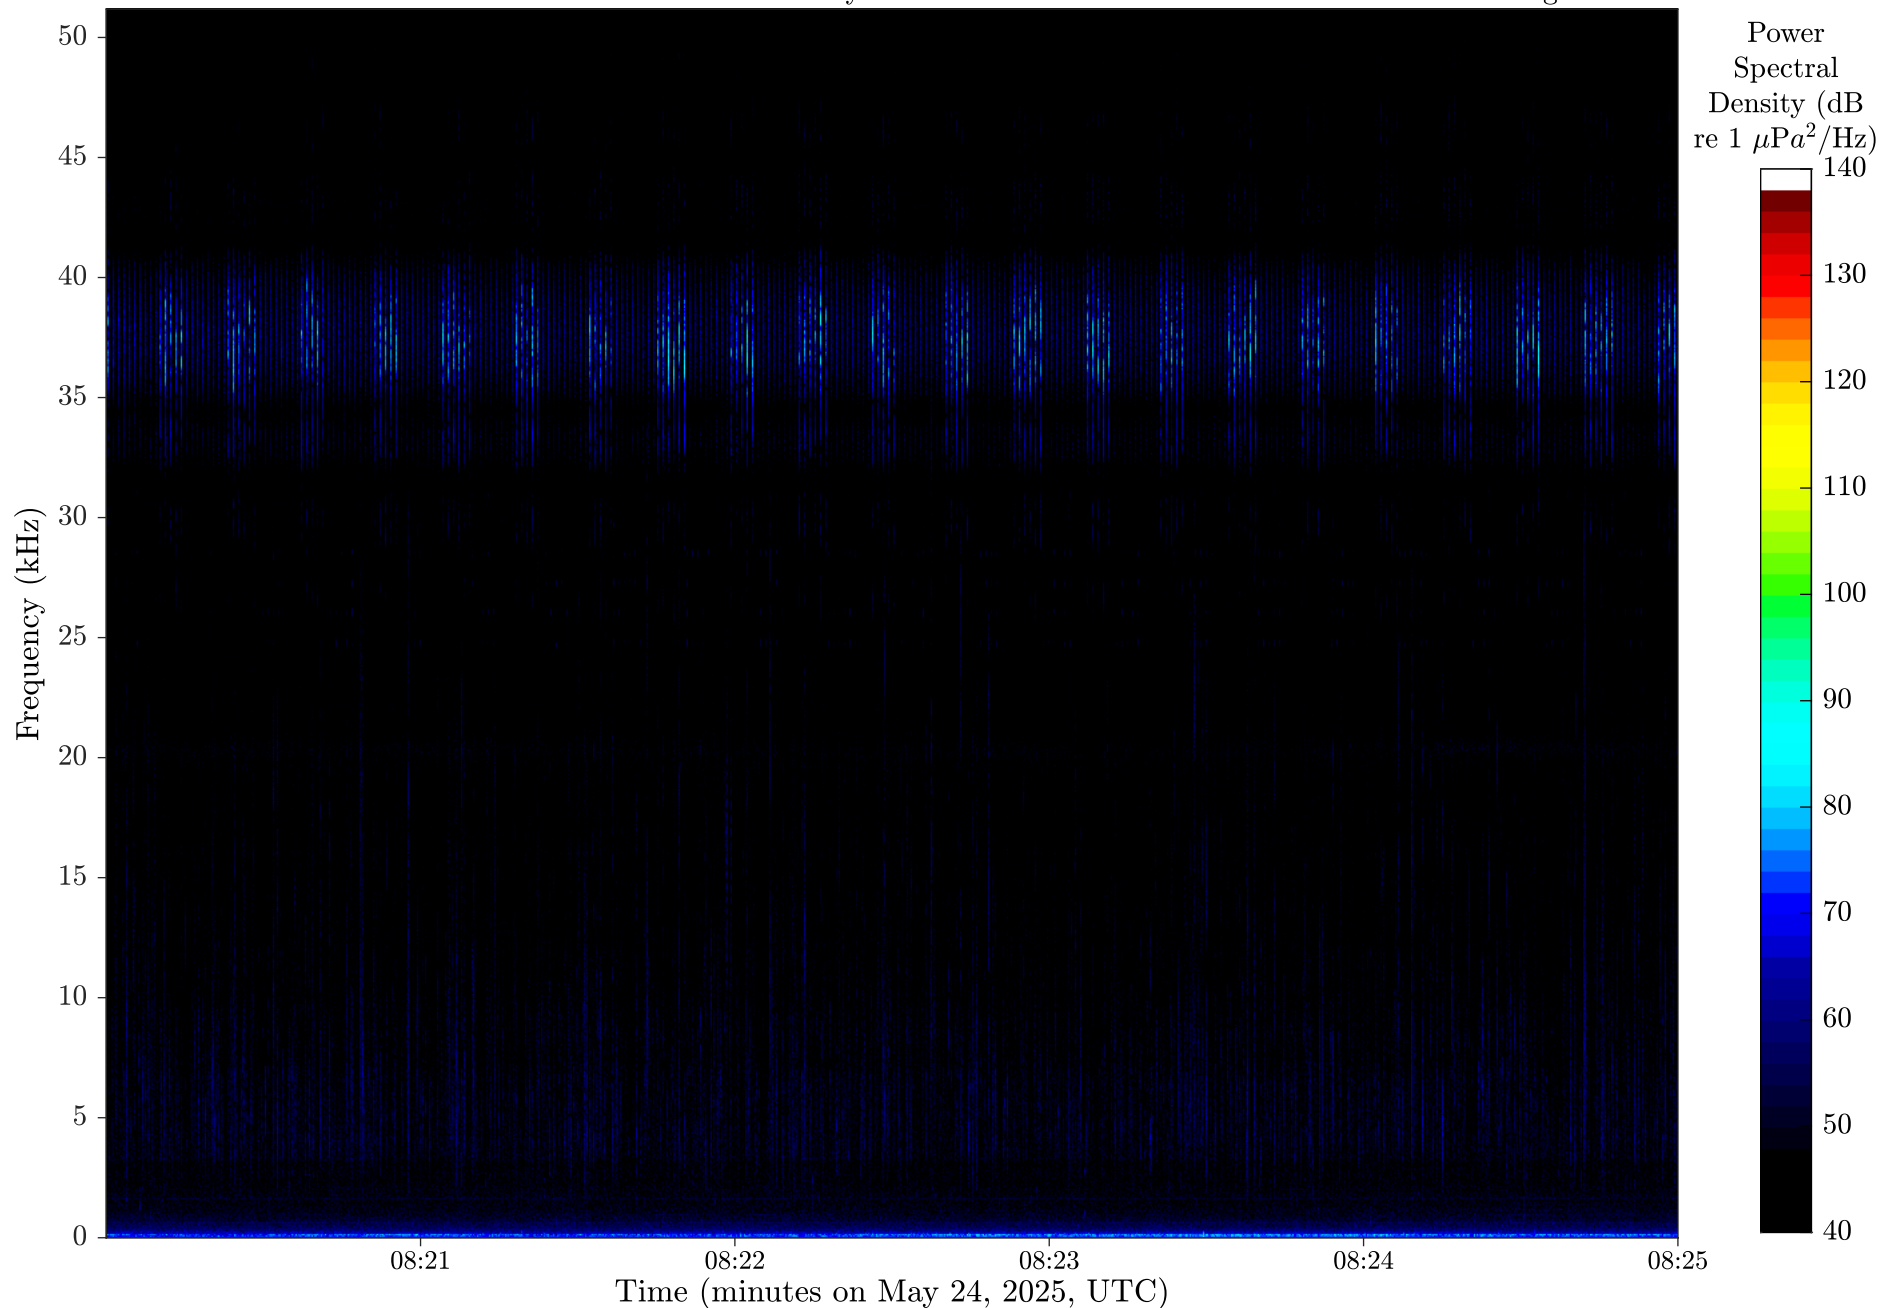


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:58 UTC

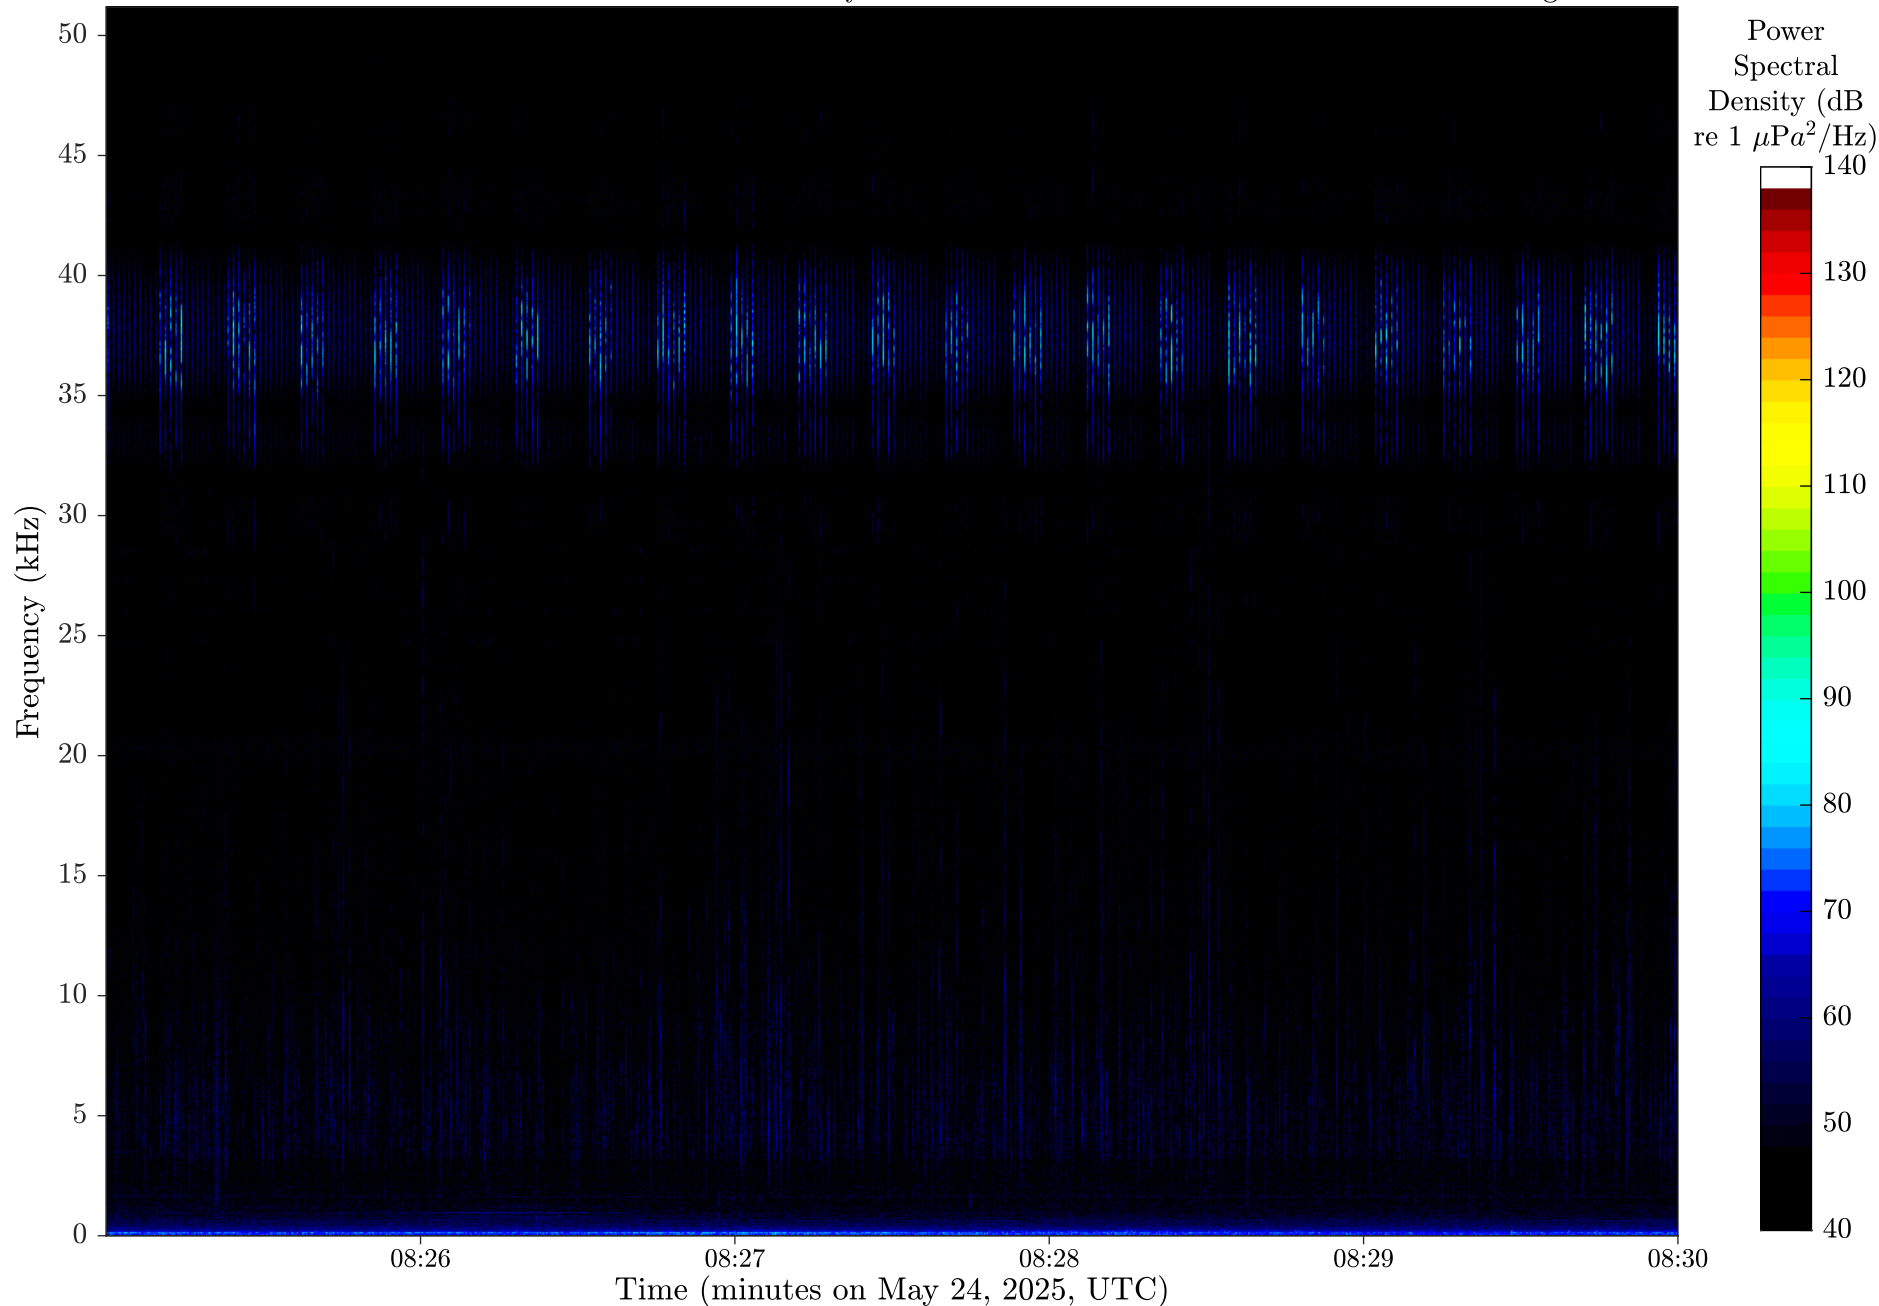


Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:06 UTC

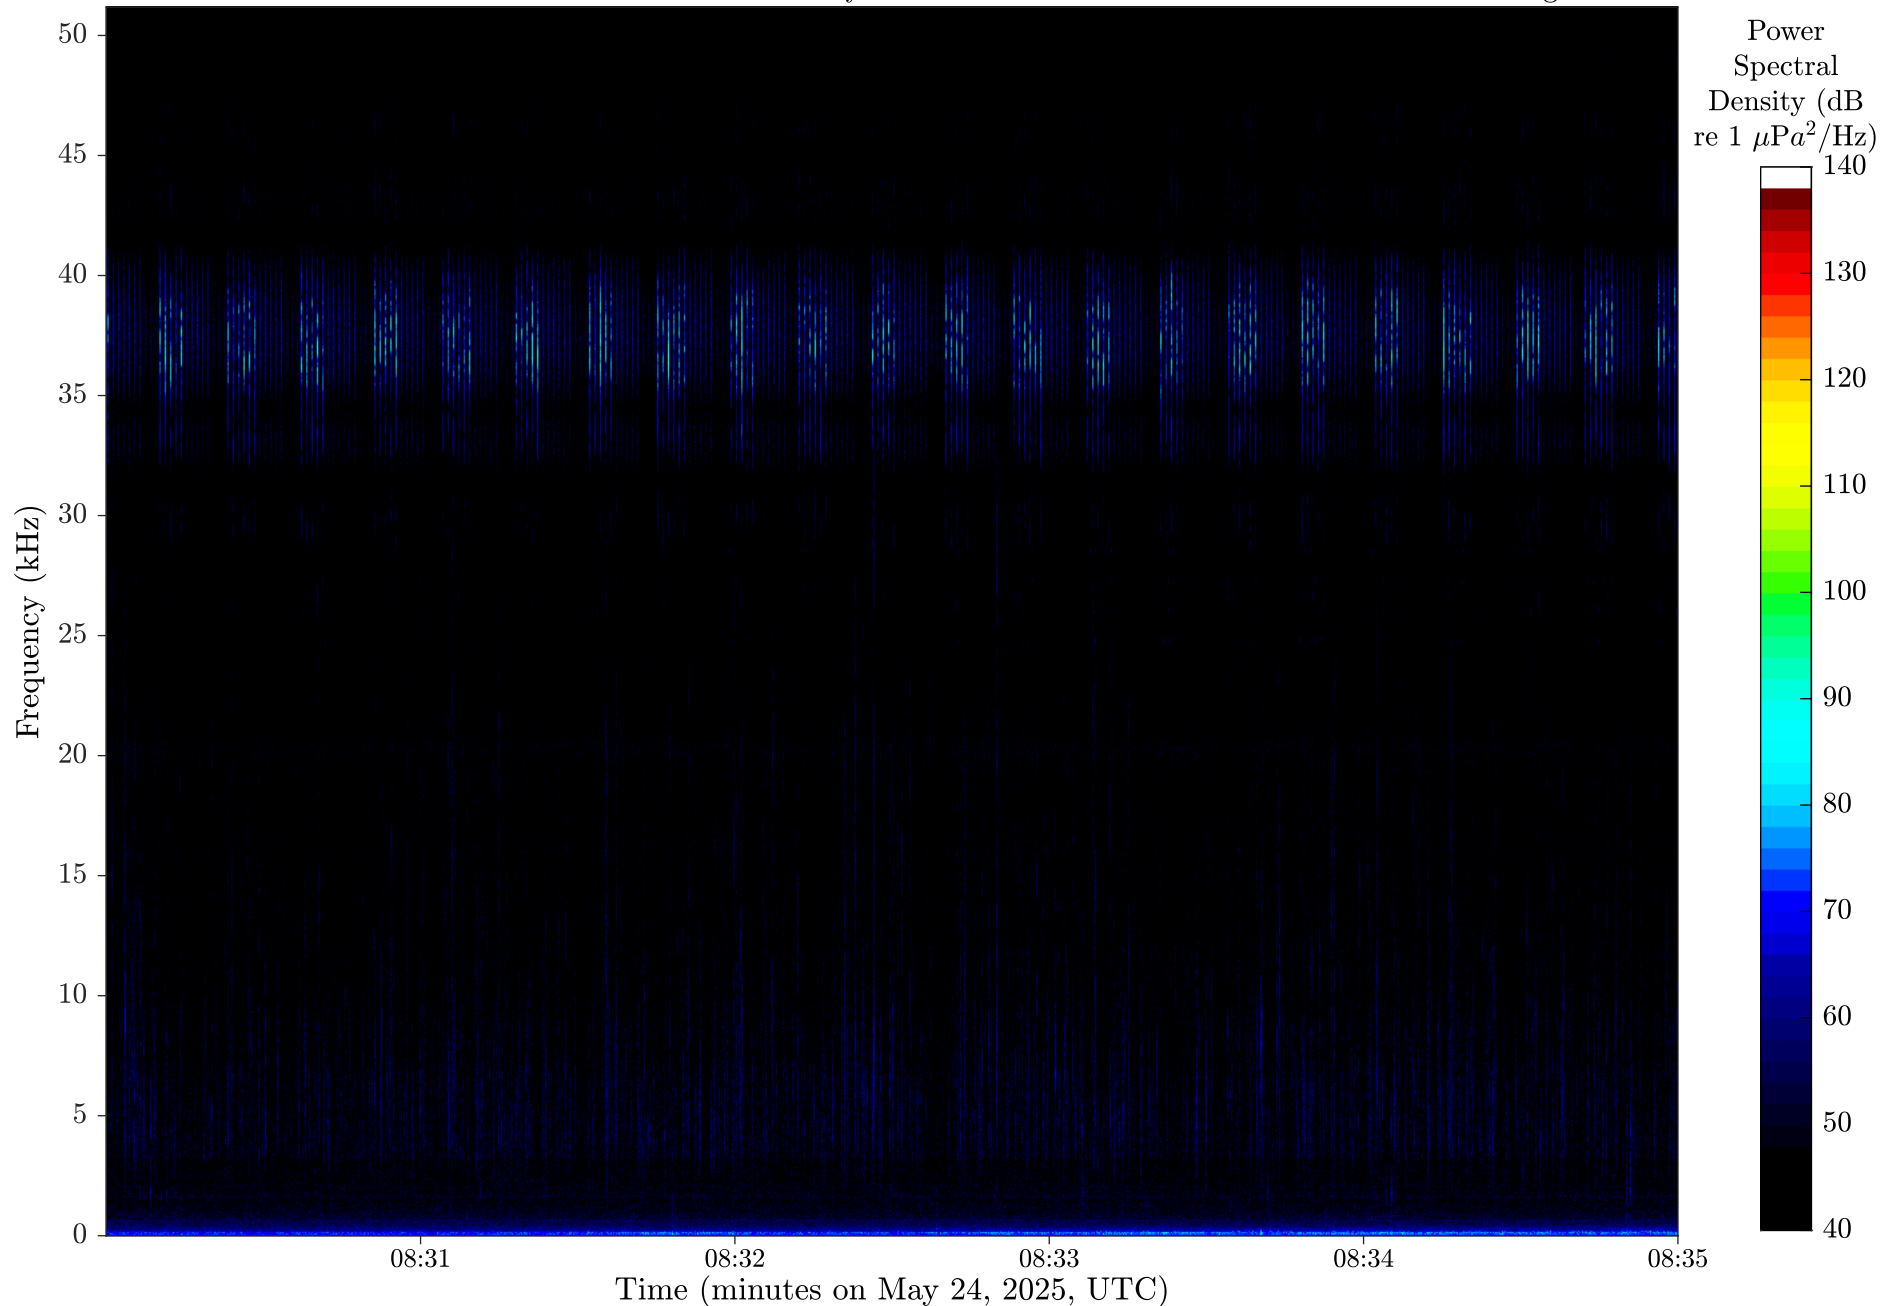


Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:14 UTC

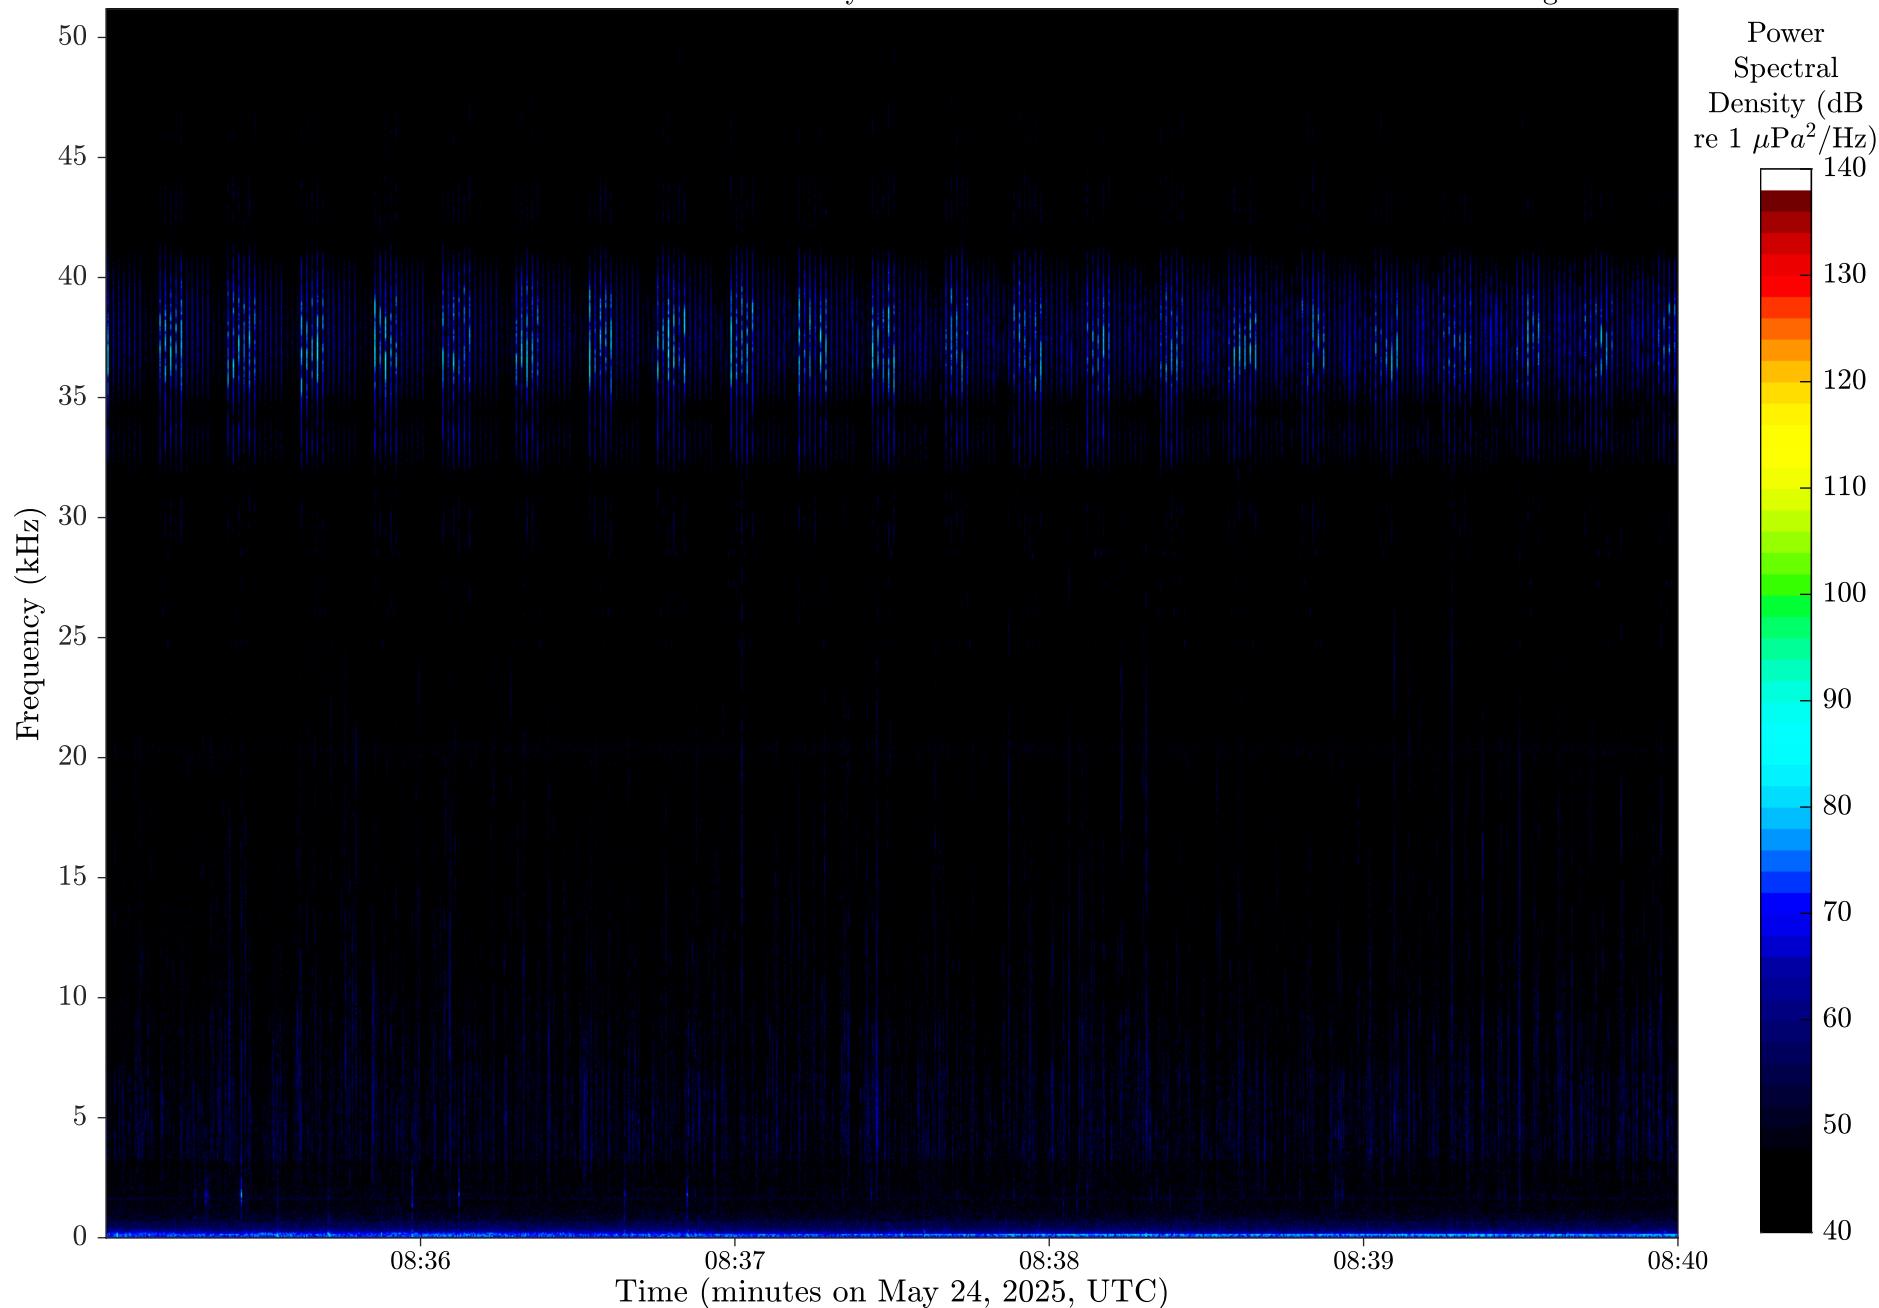


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:21:22 UTC

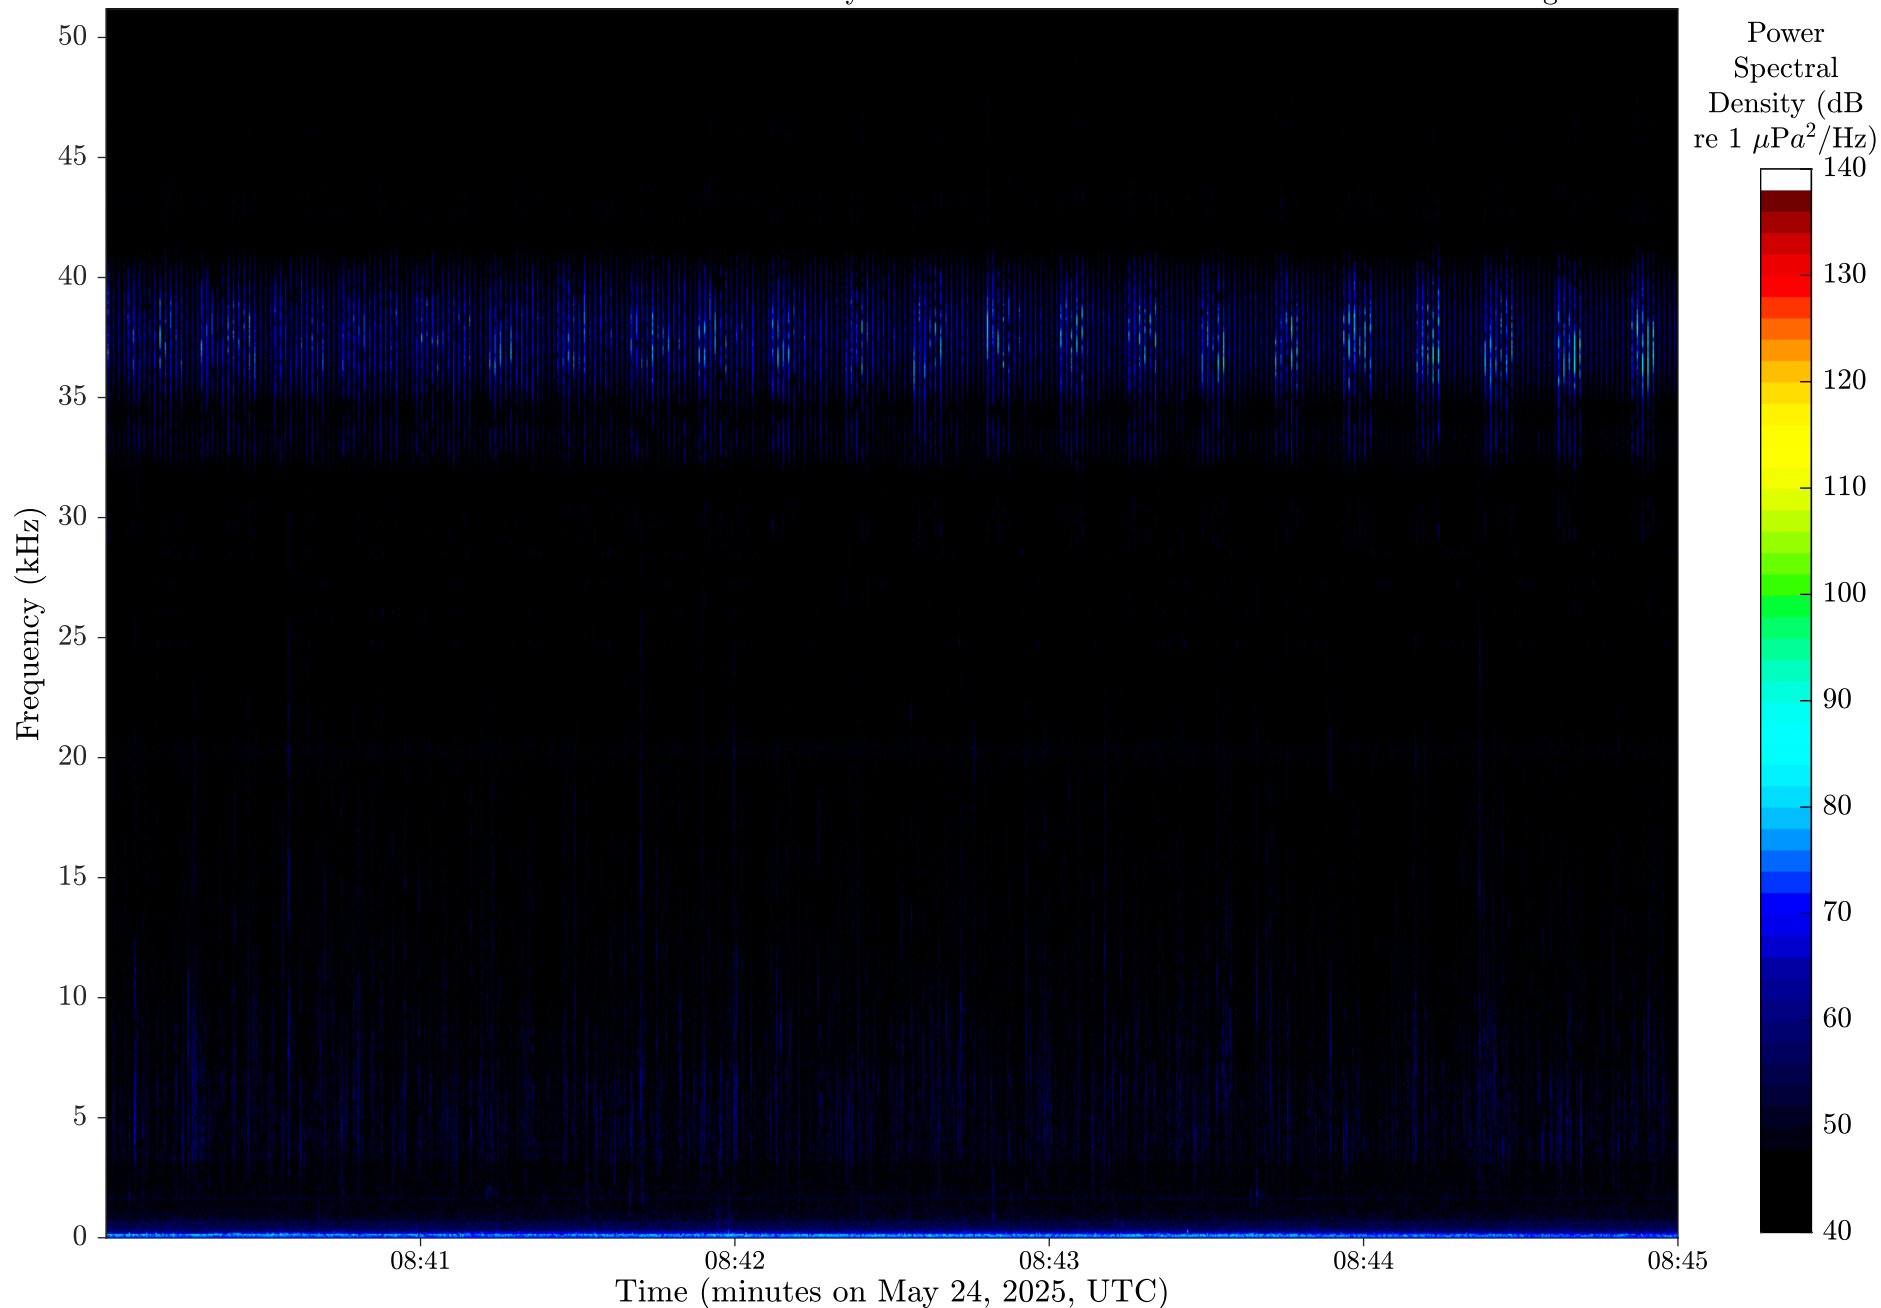

Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:21:30 UTC

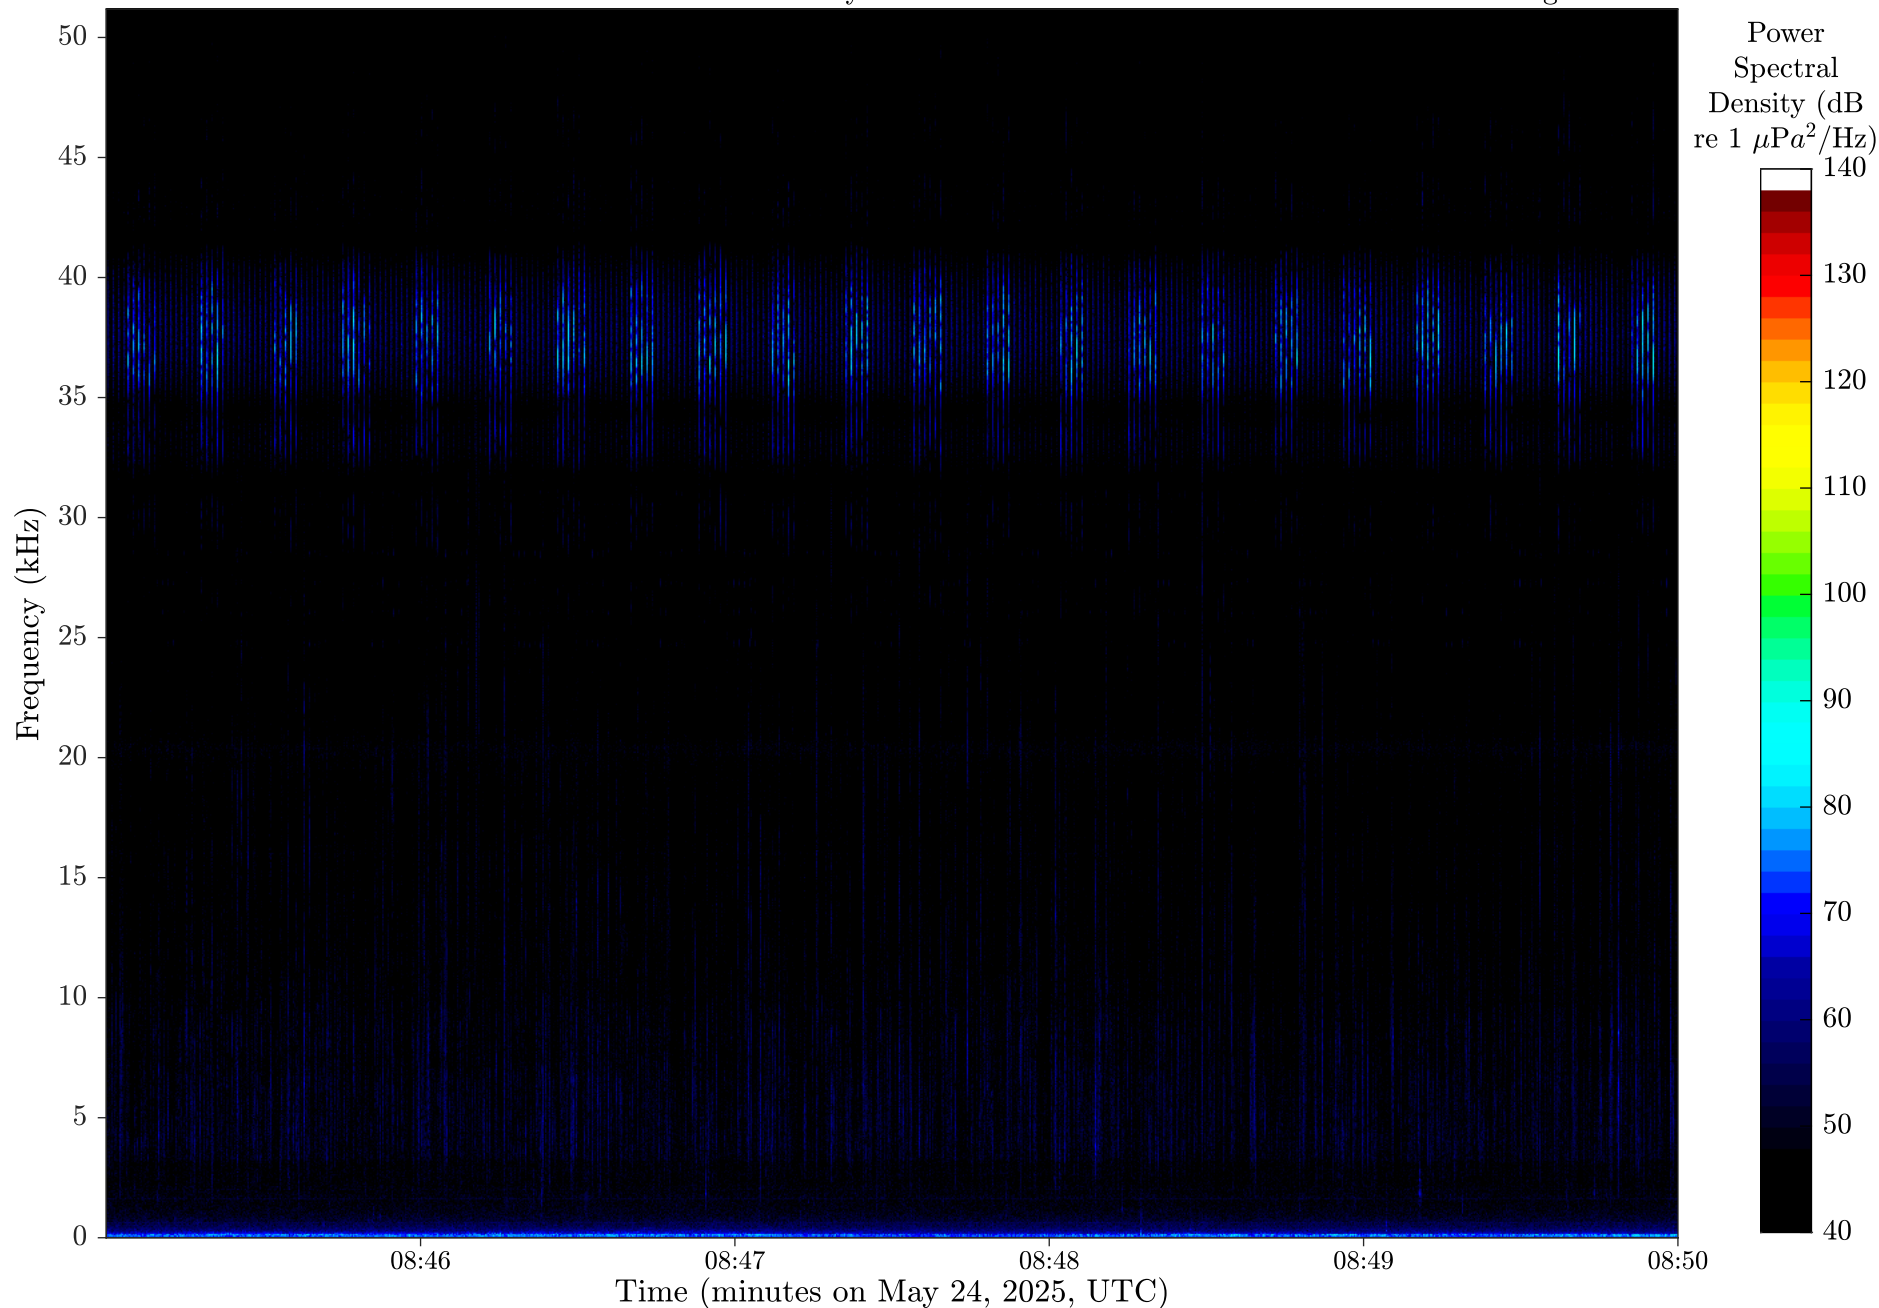

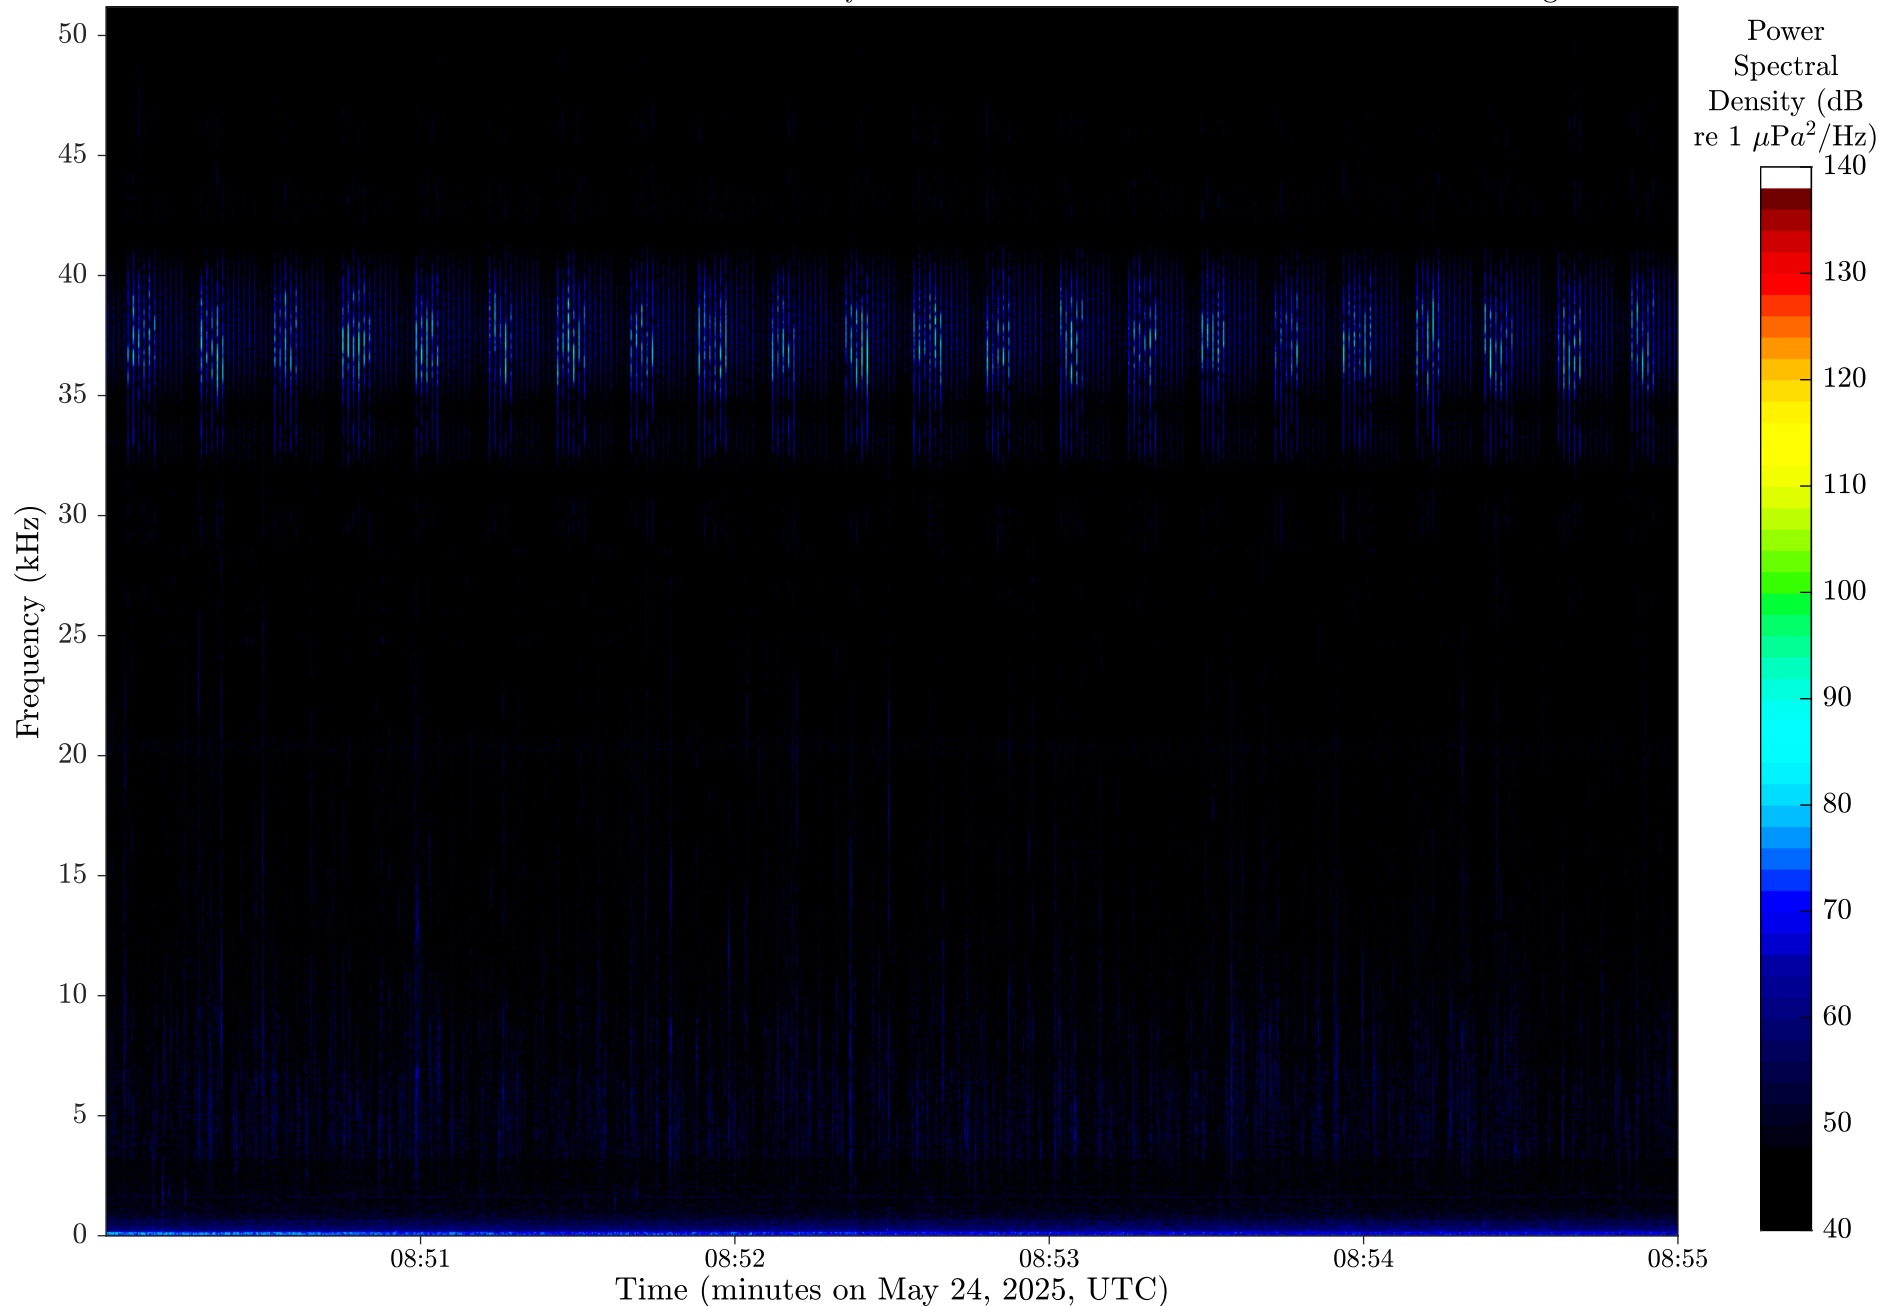


Comments: 36.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:46 UTC

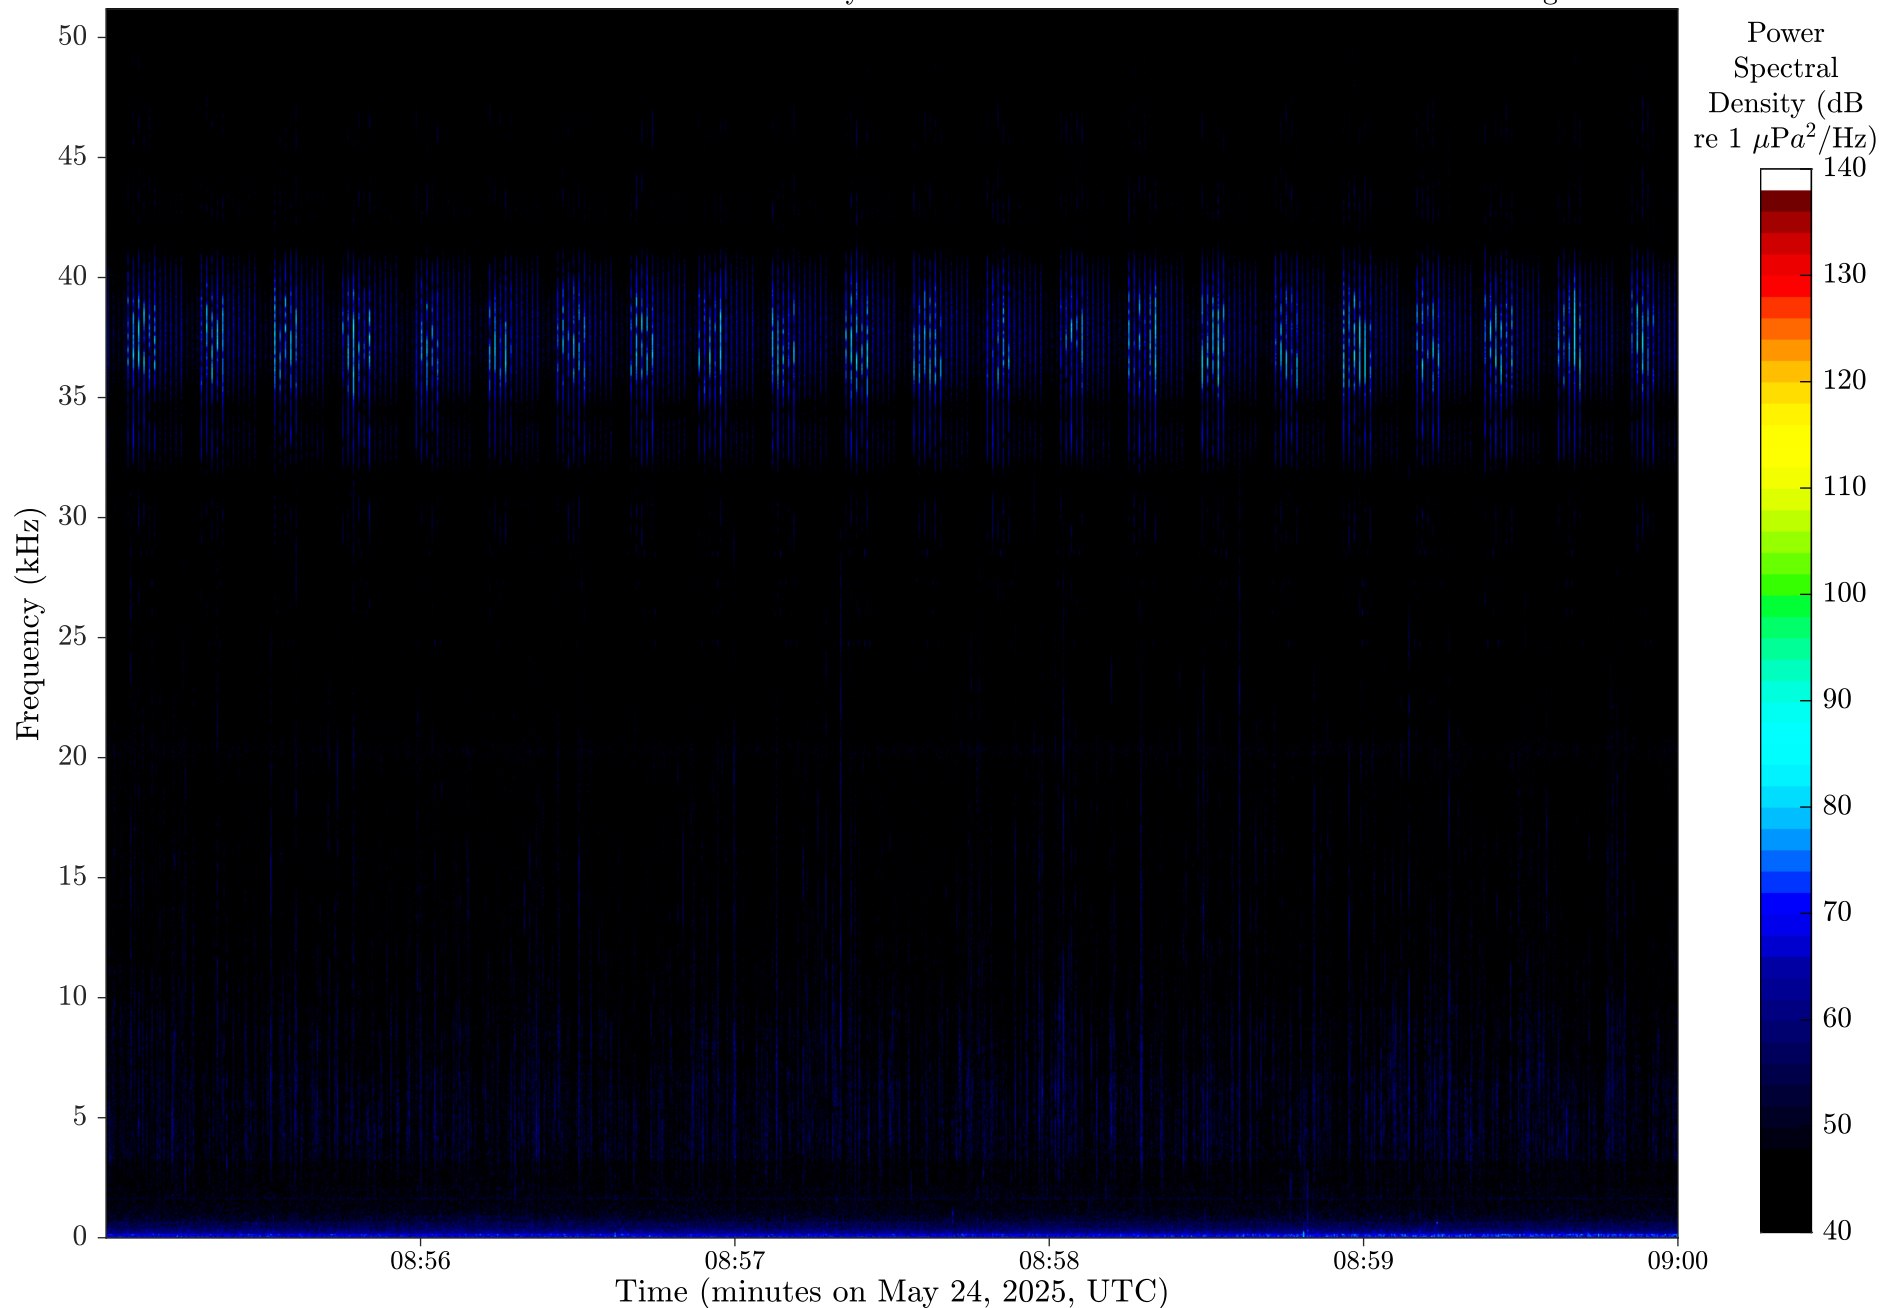


Comments: 36.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:54 UTC

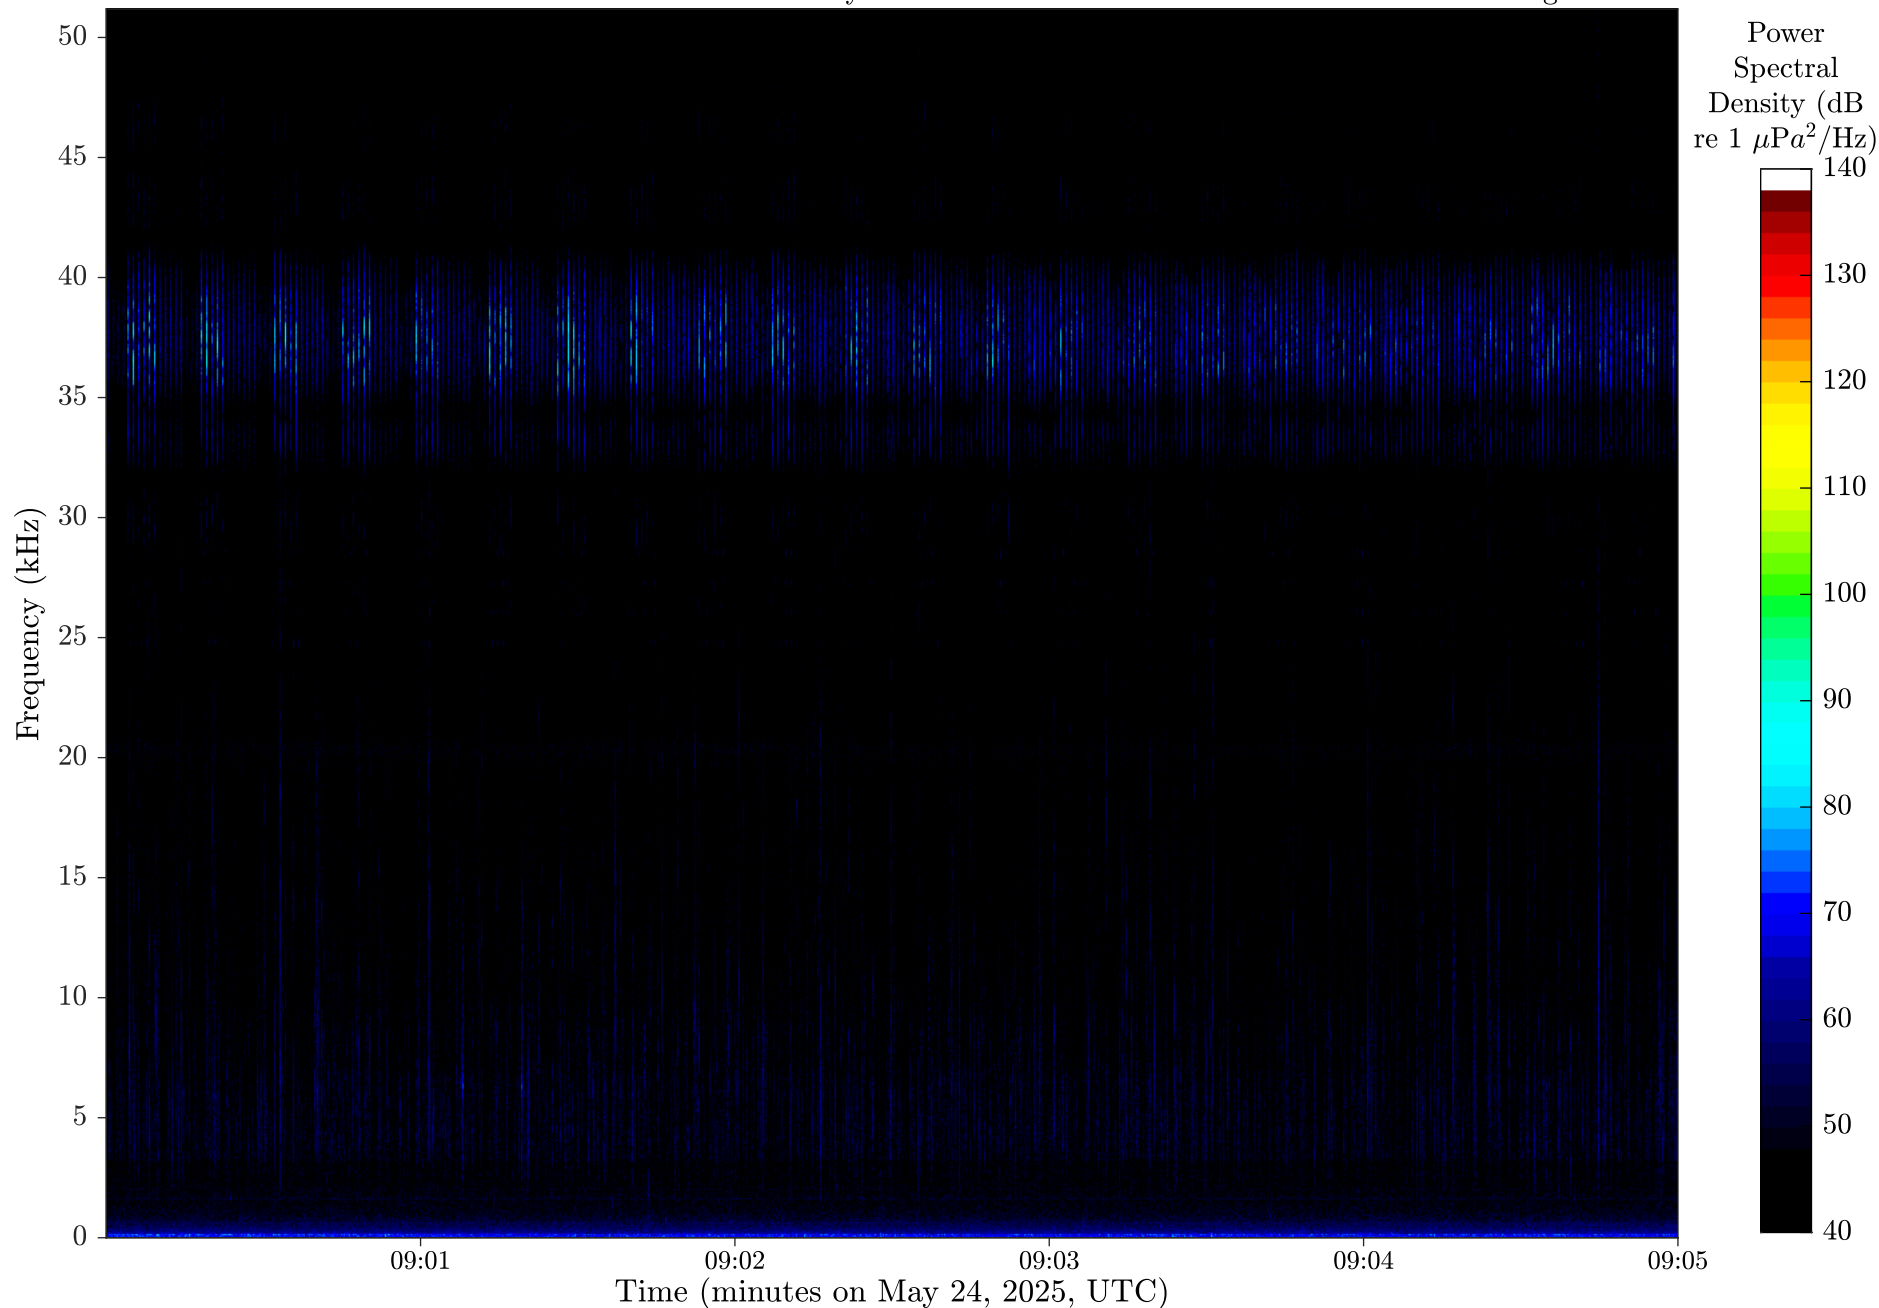


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:02 UTC

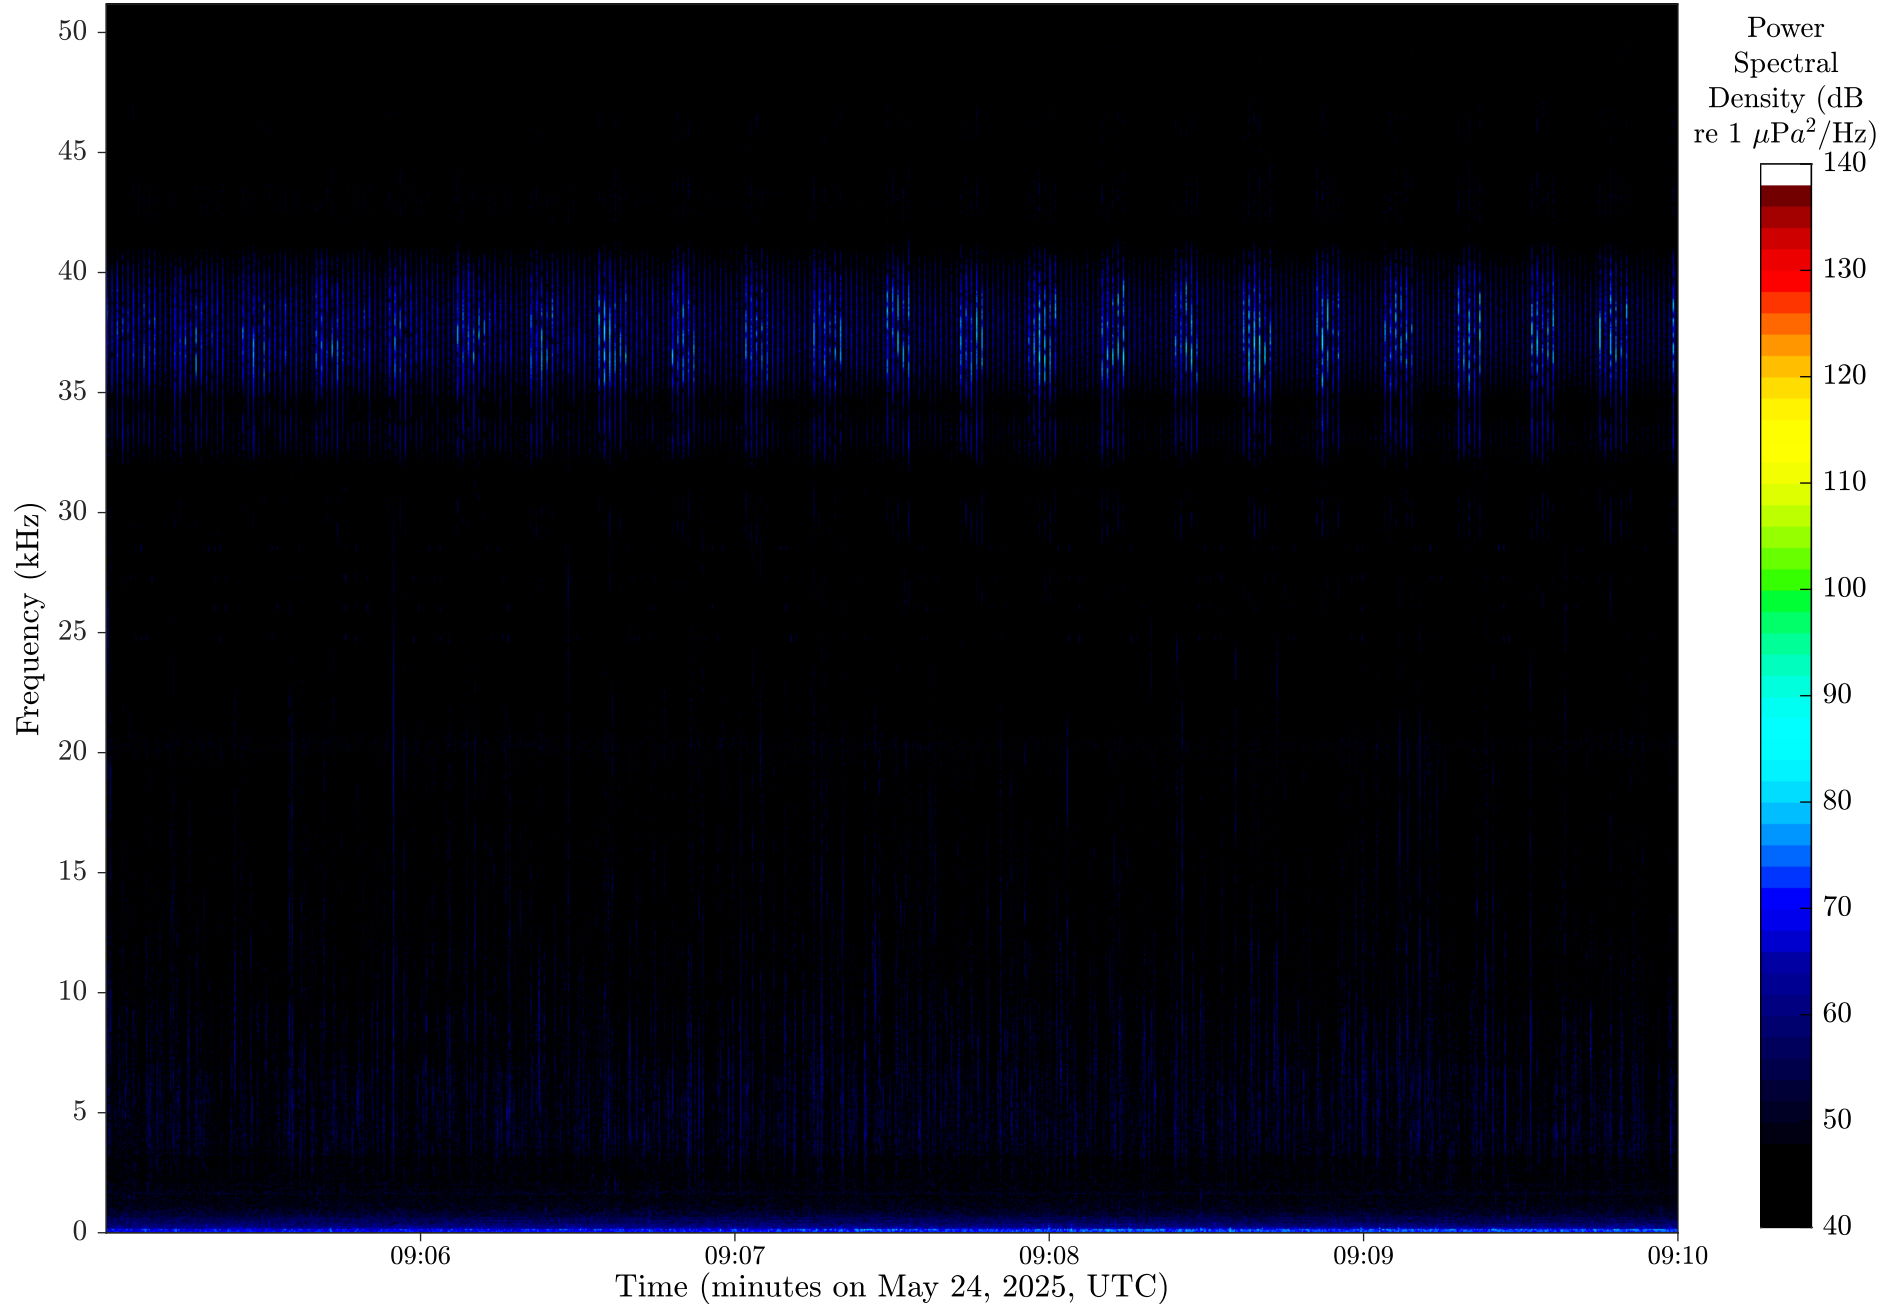


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:12 UTC

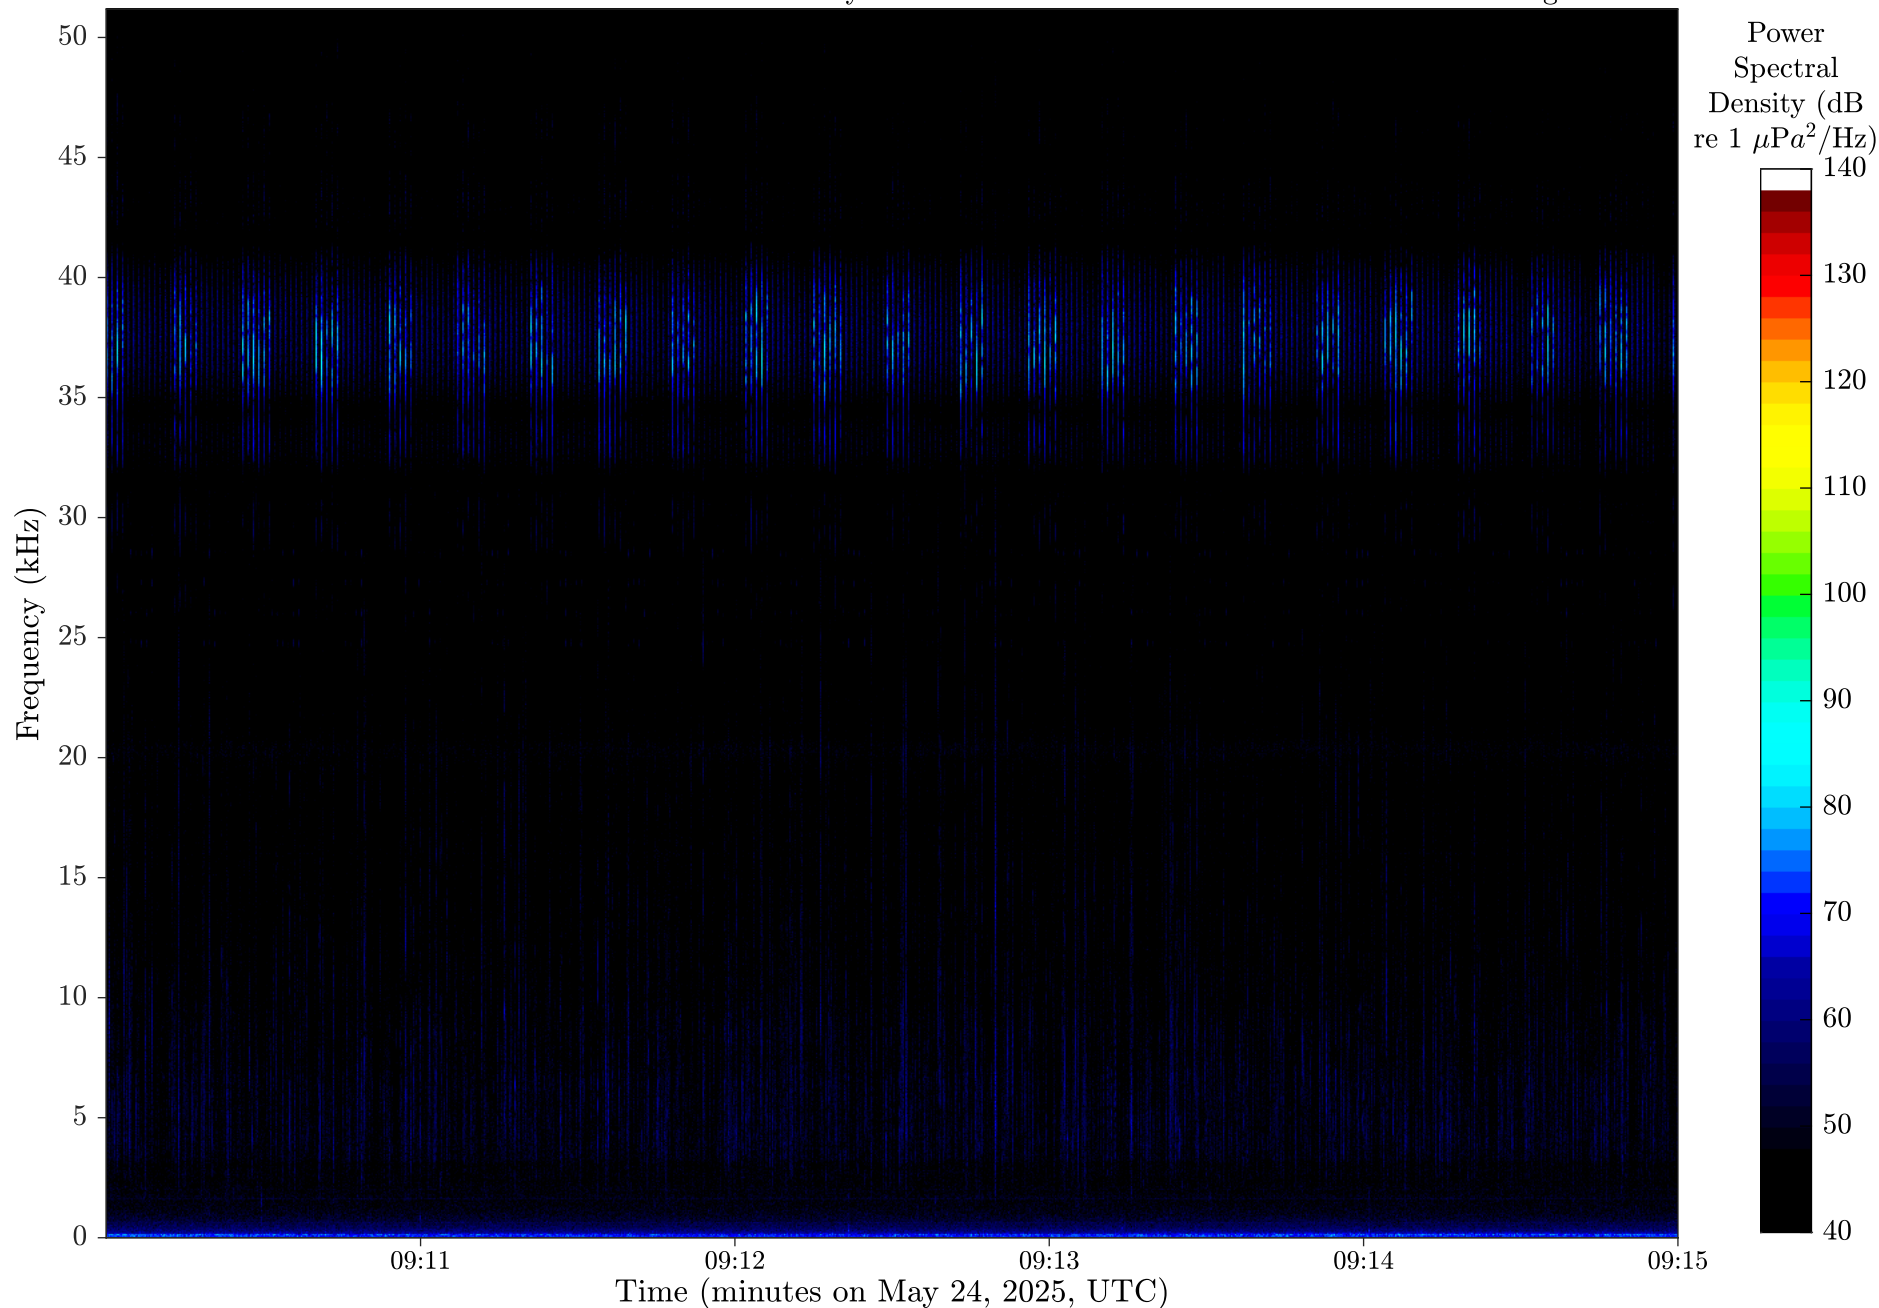


Comments: 35.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:22:22 UTC

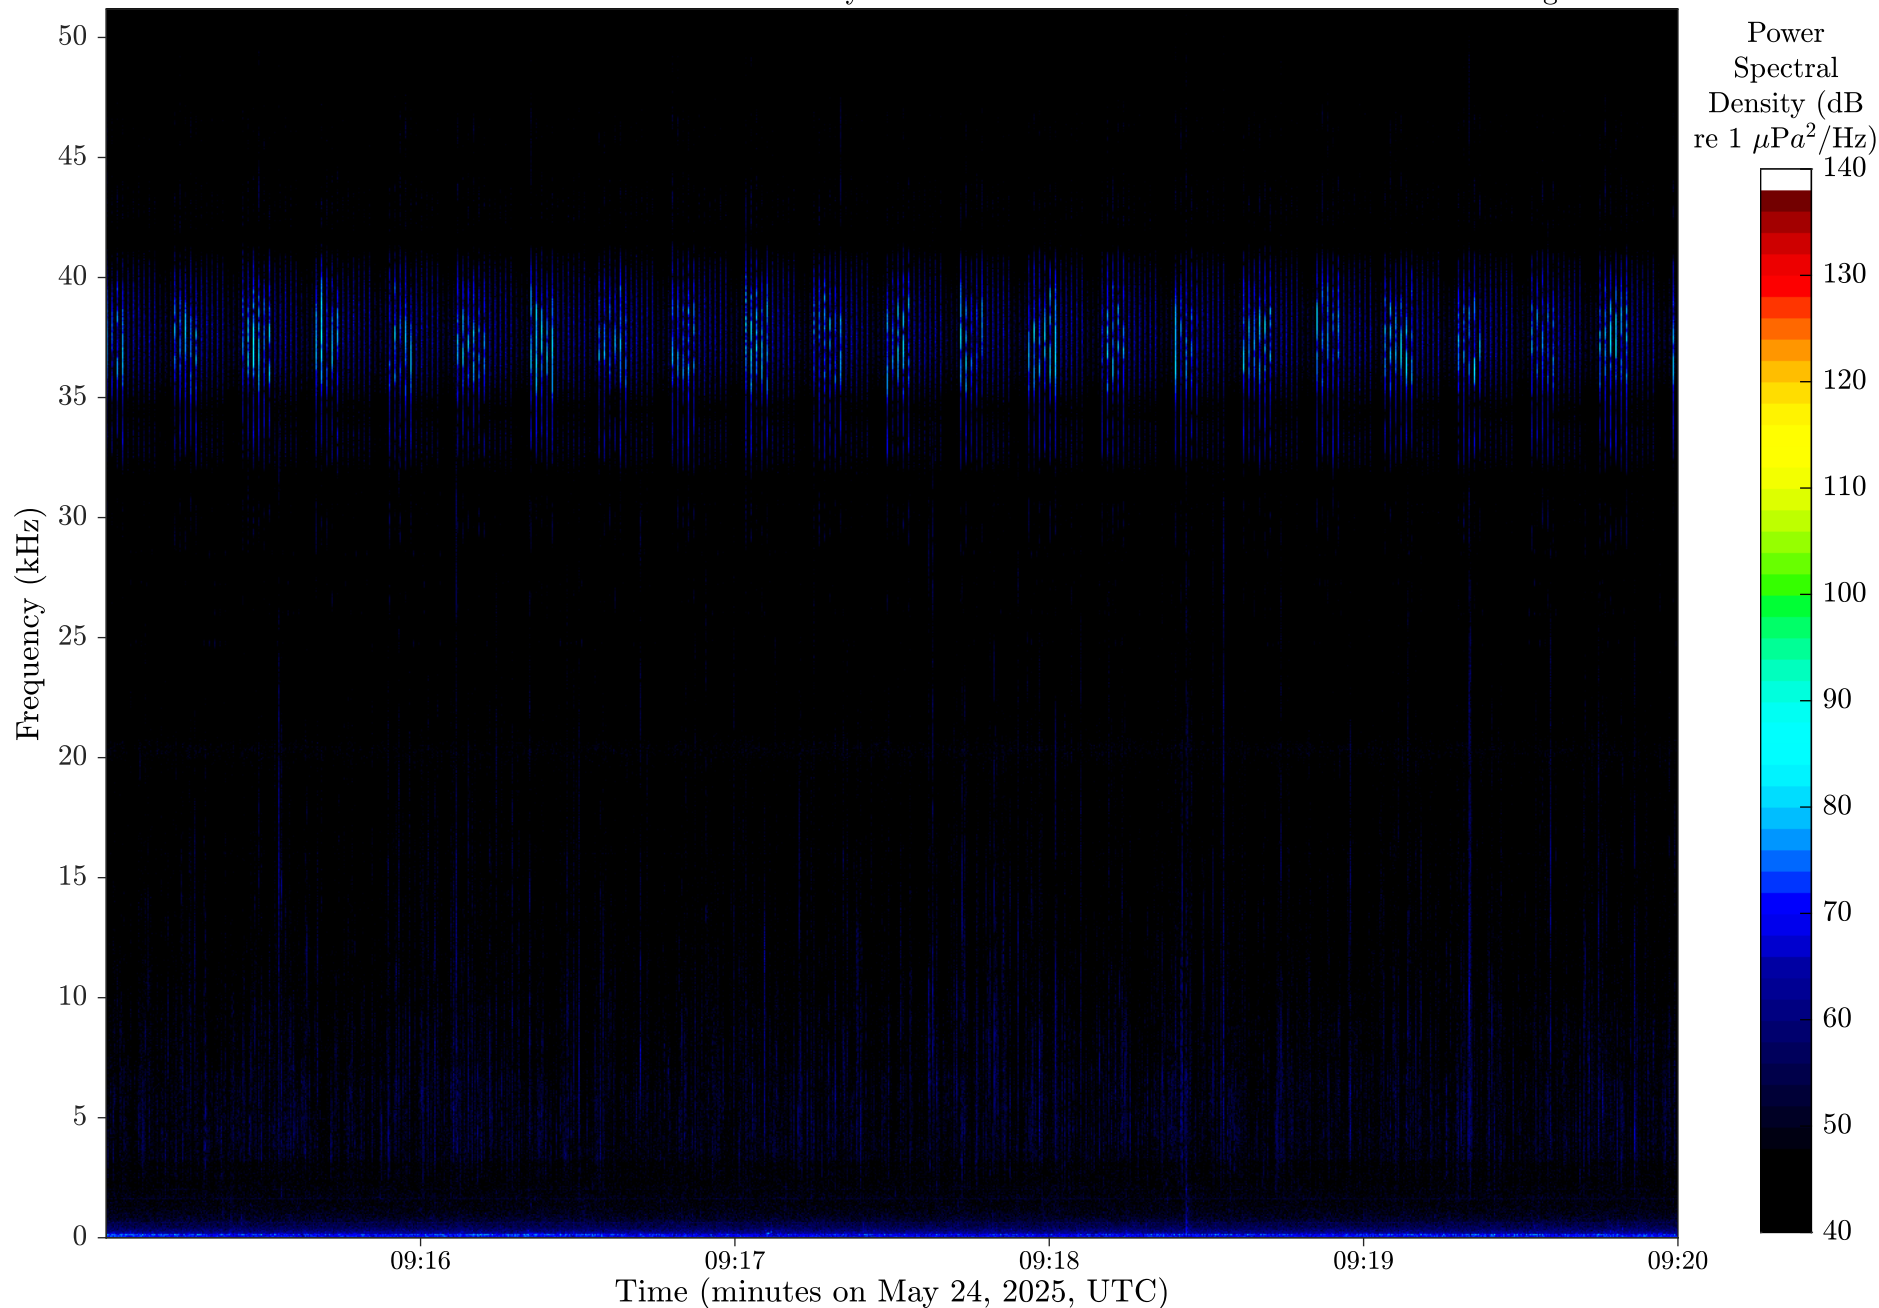

Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:22:31 UTC

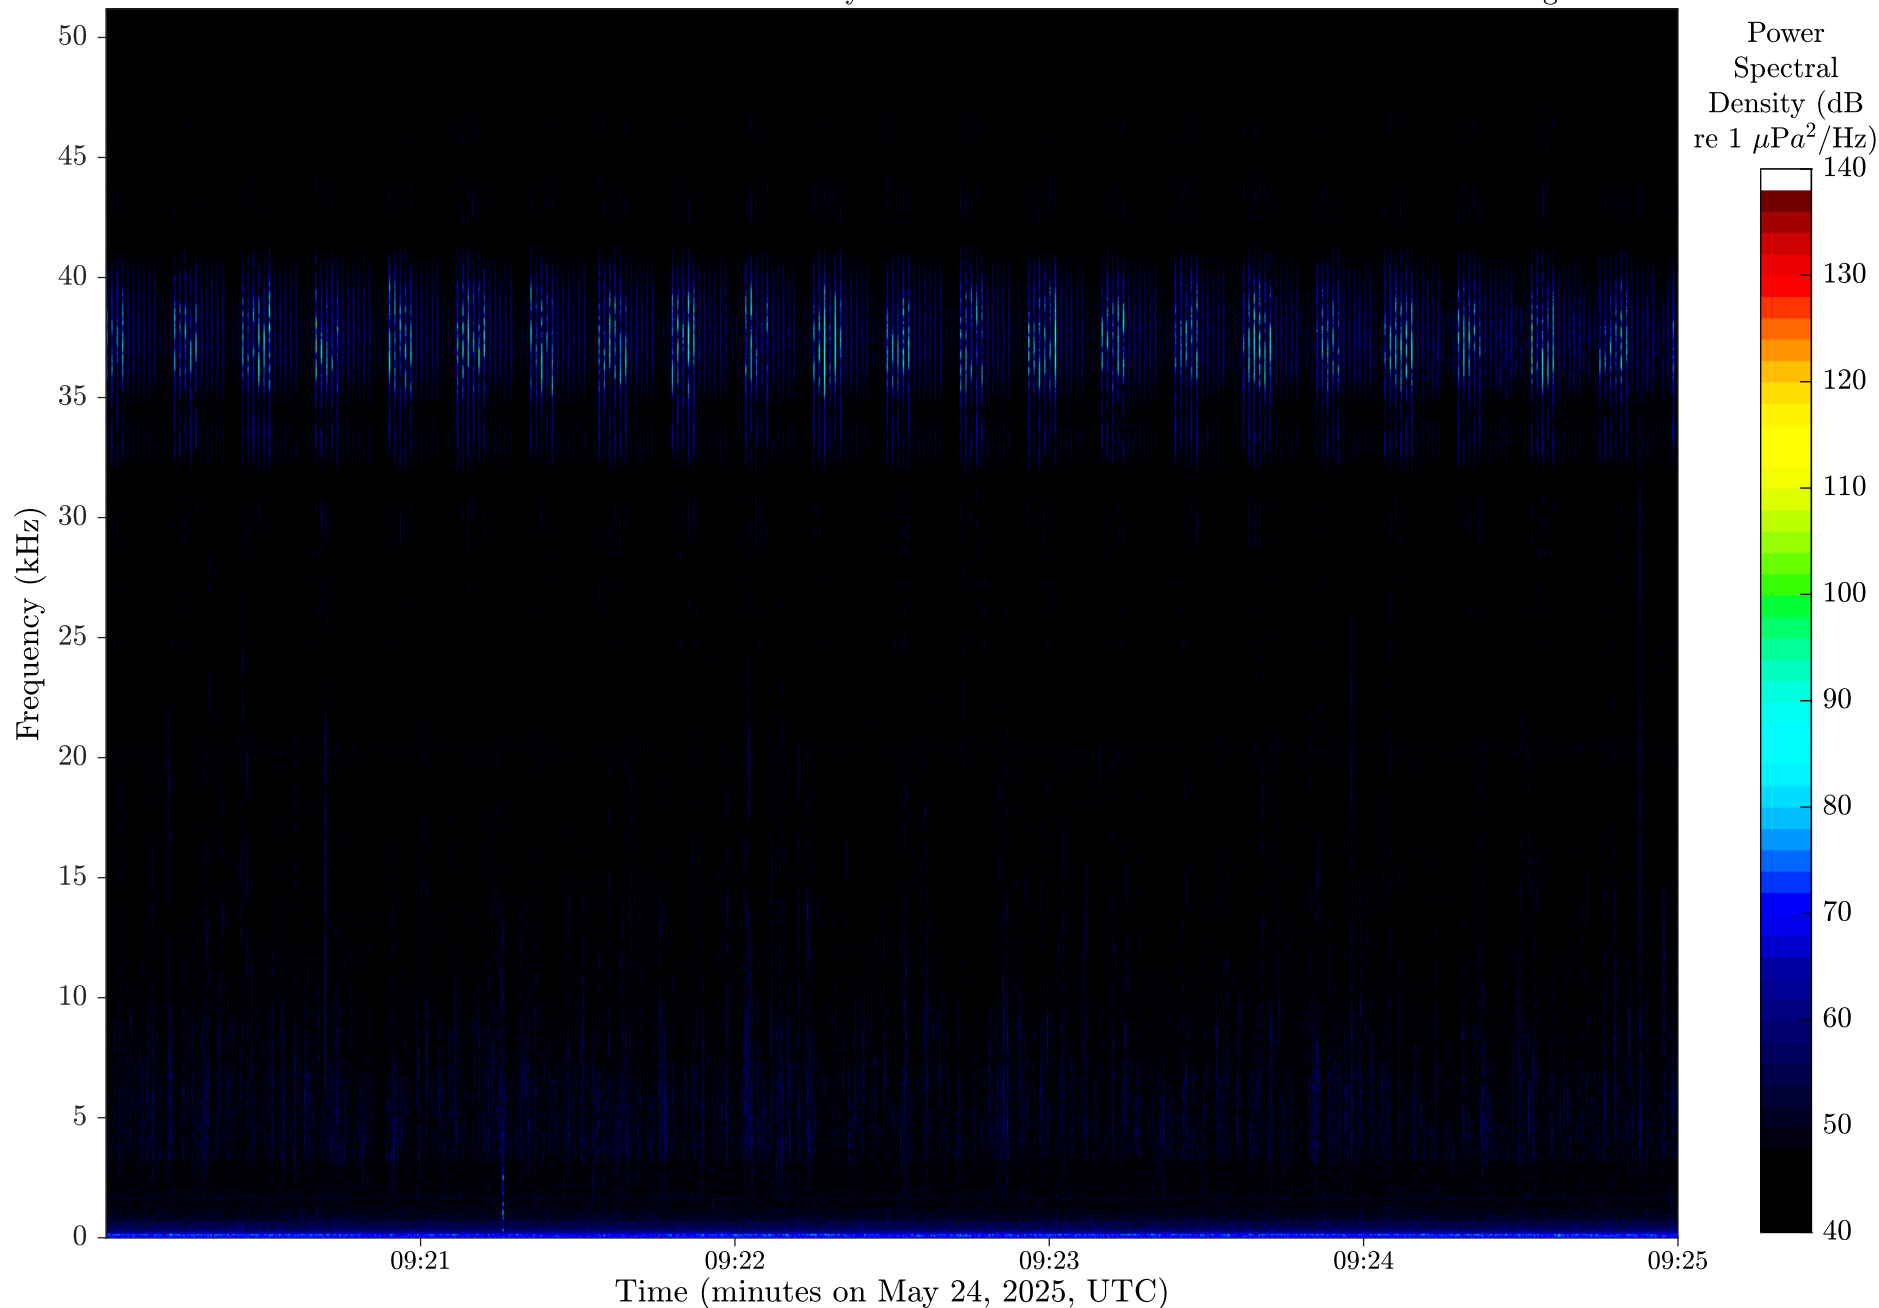

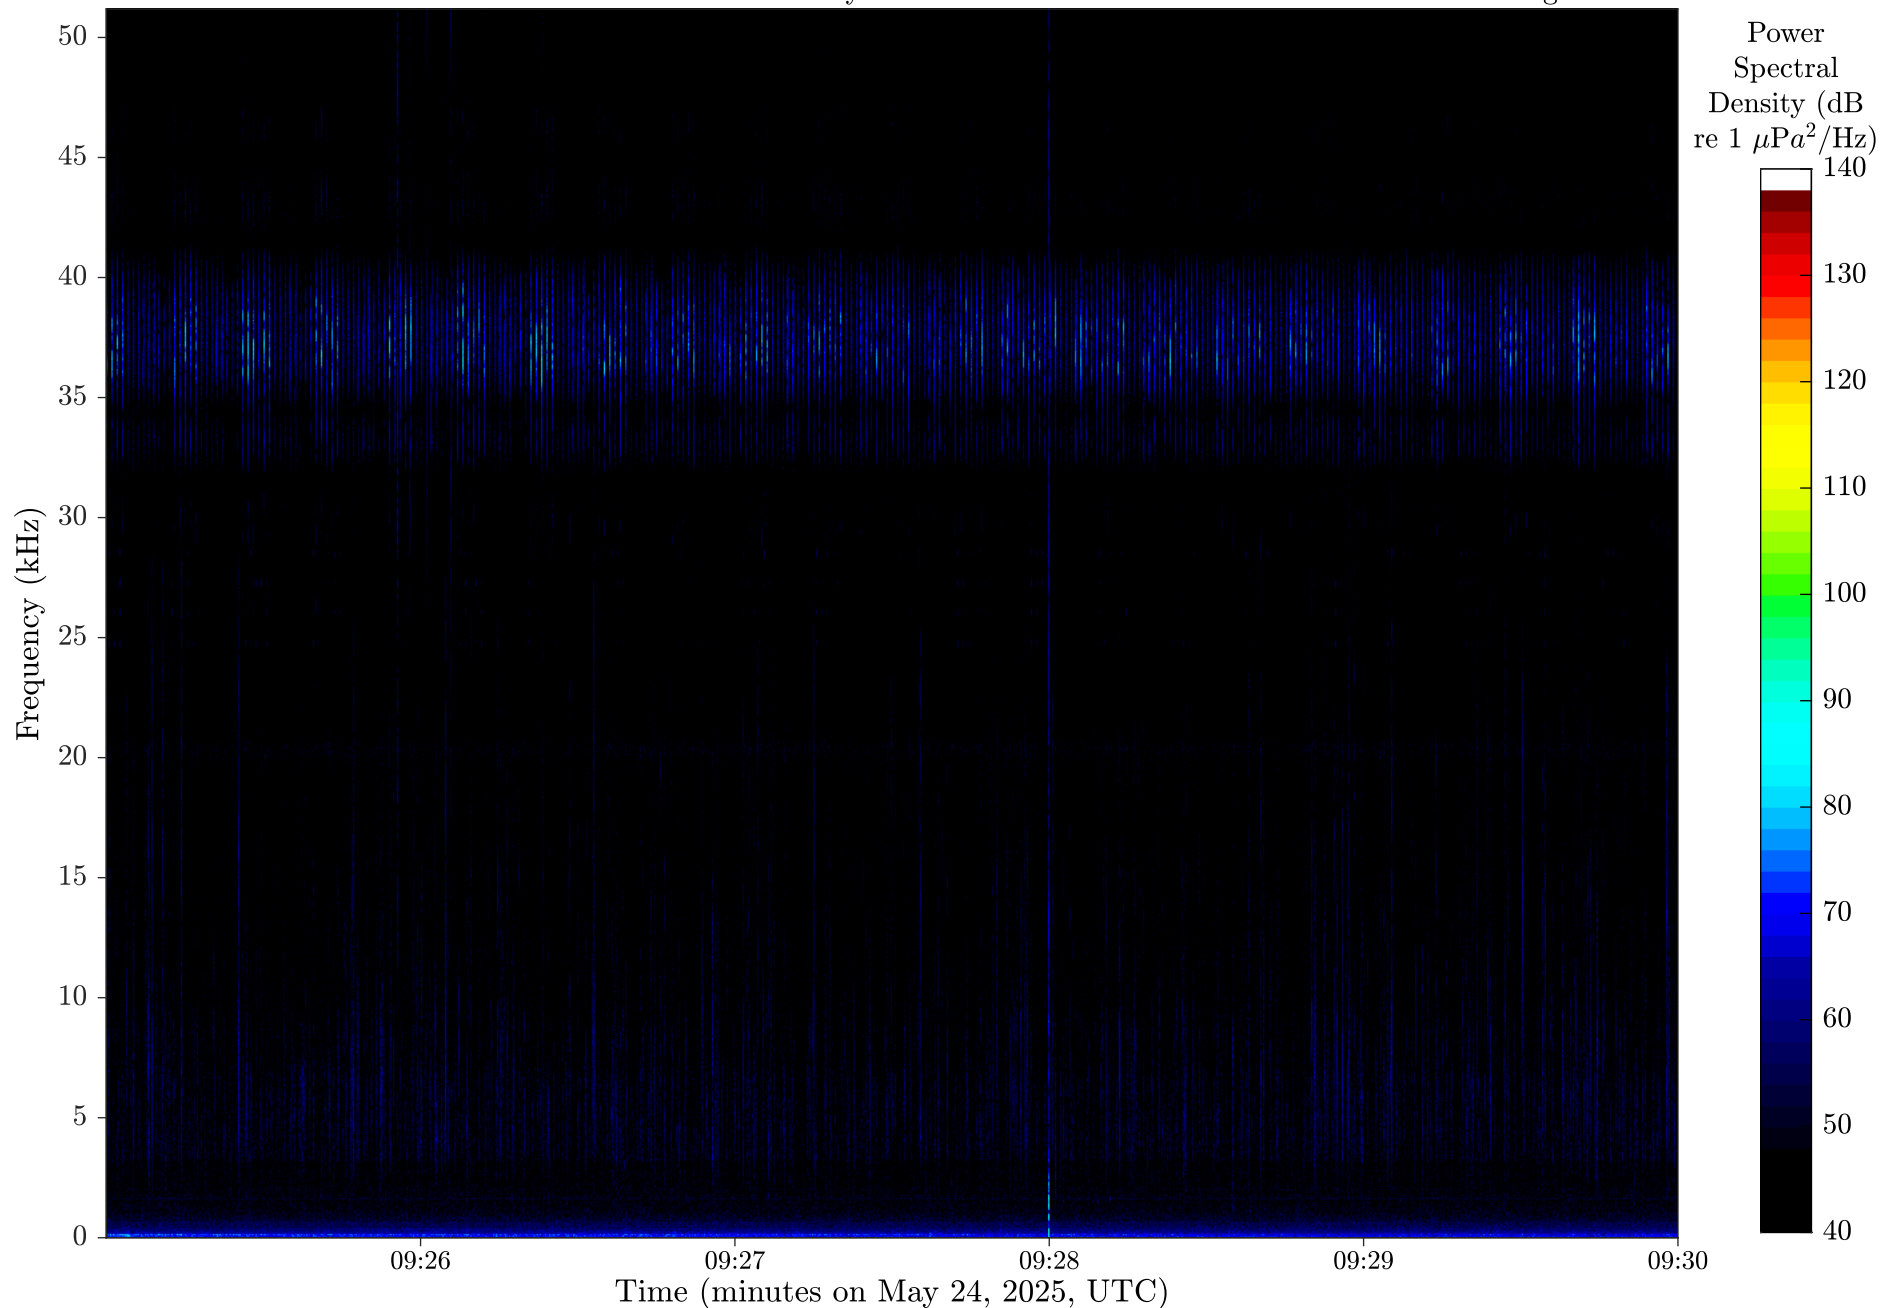


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:48 UTC

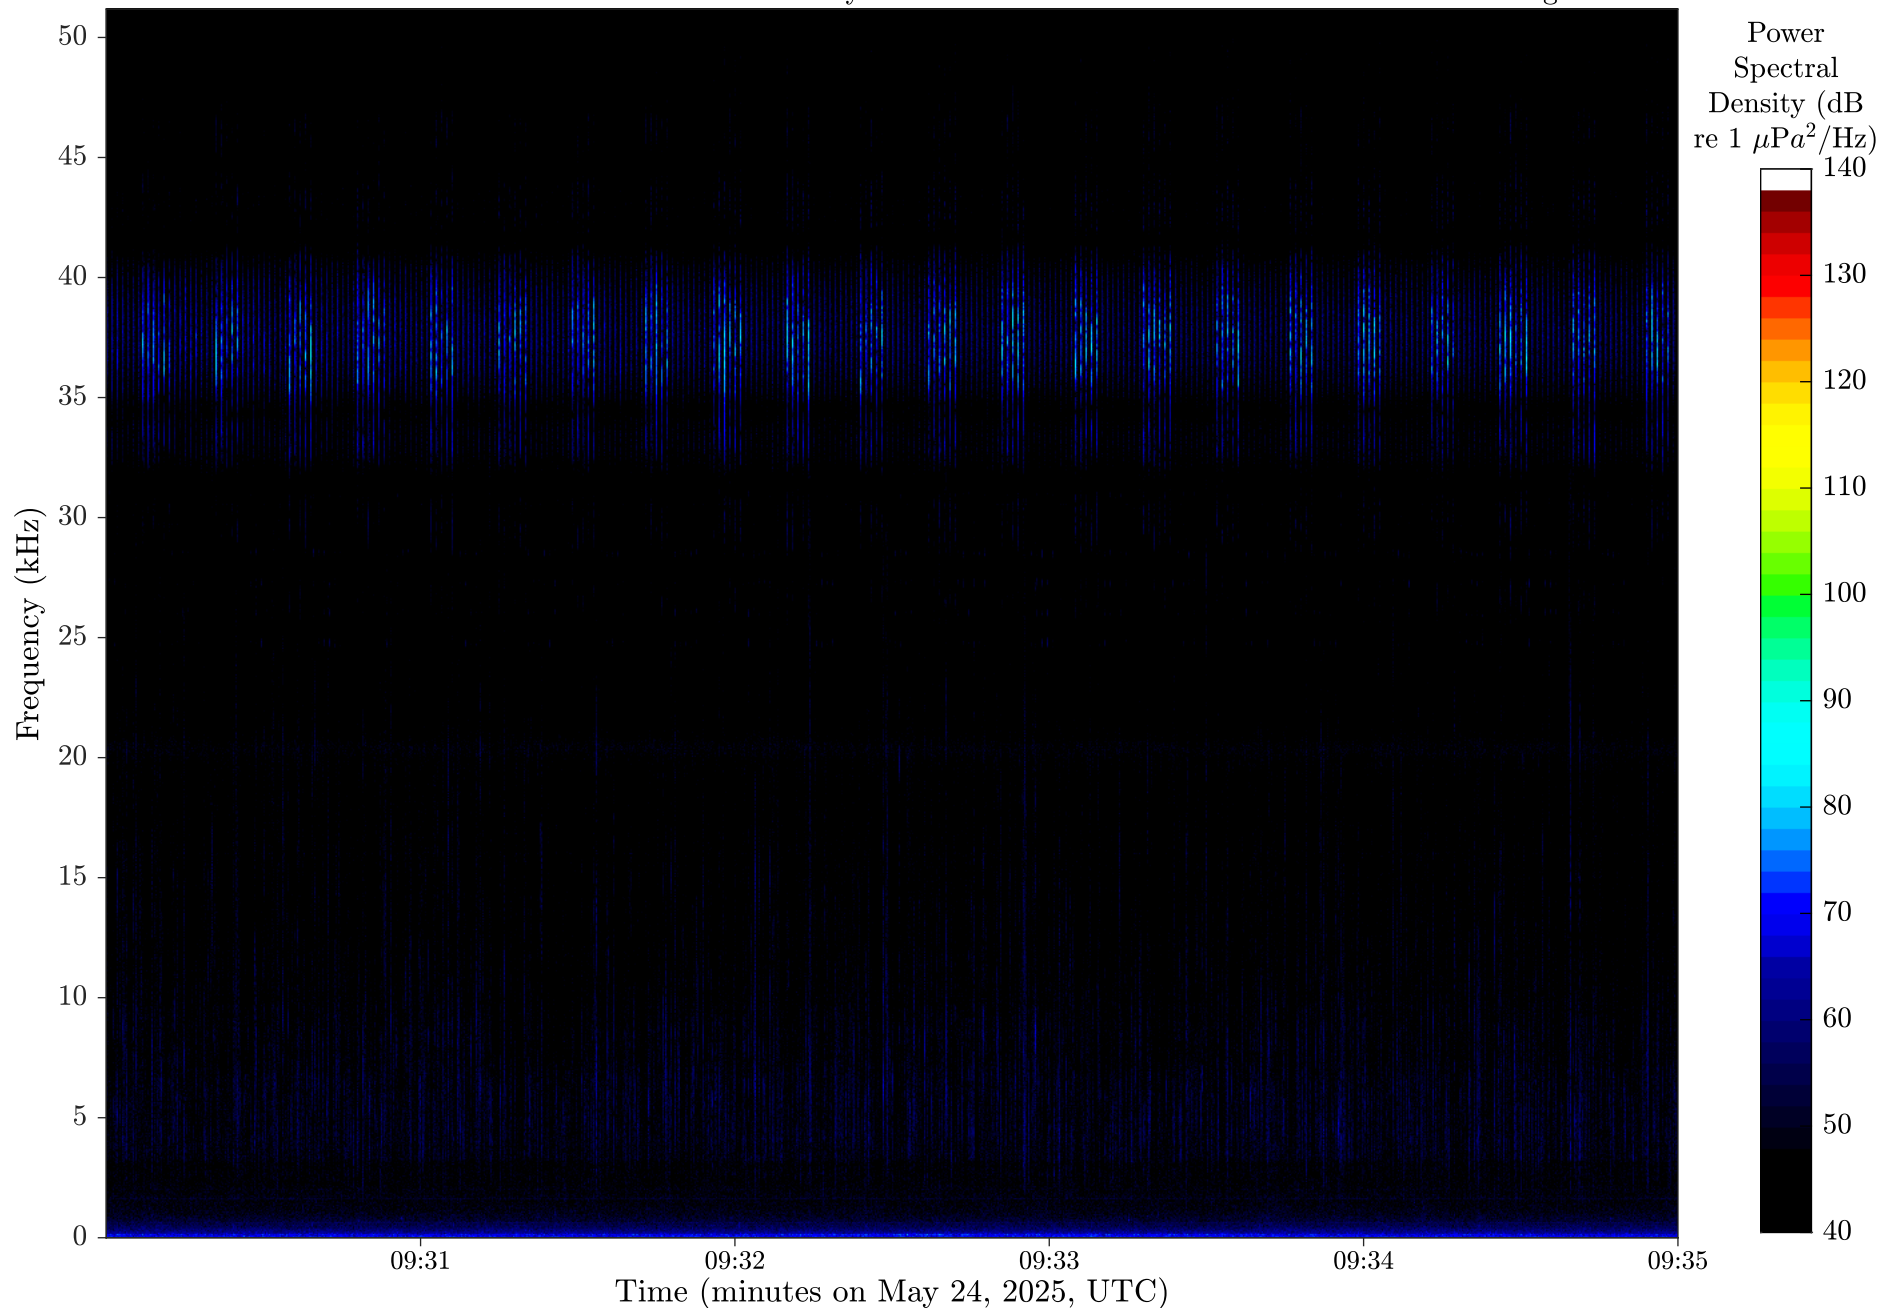


Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:58 UTC

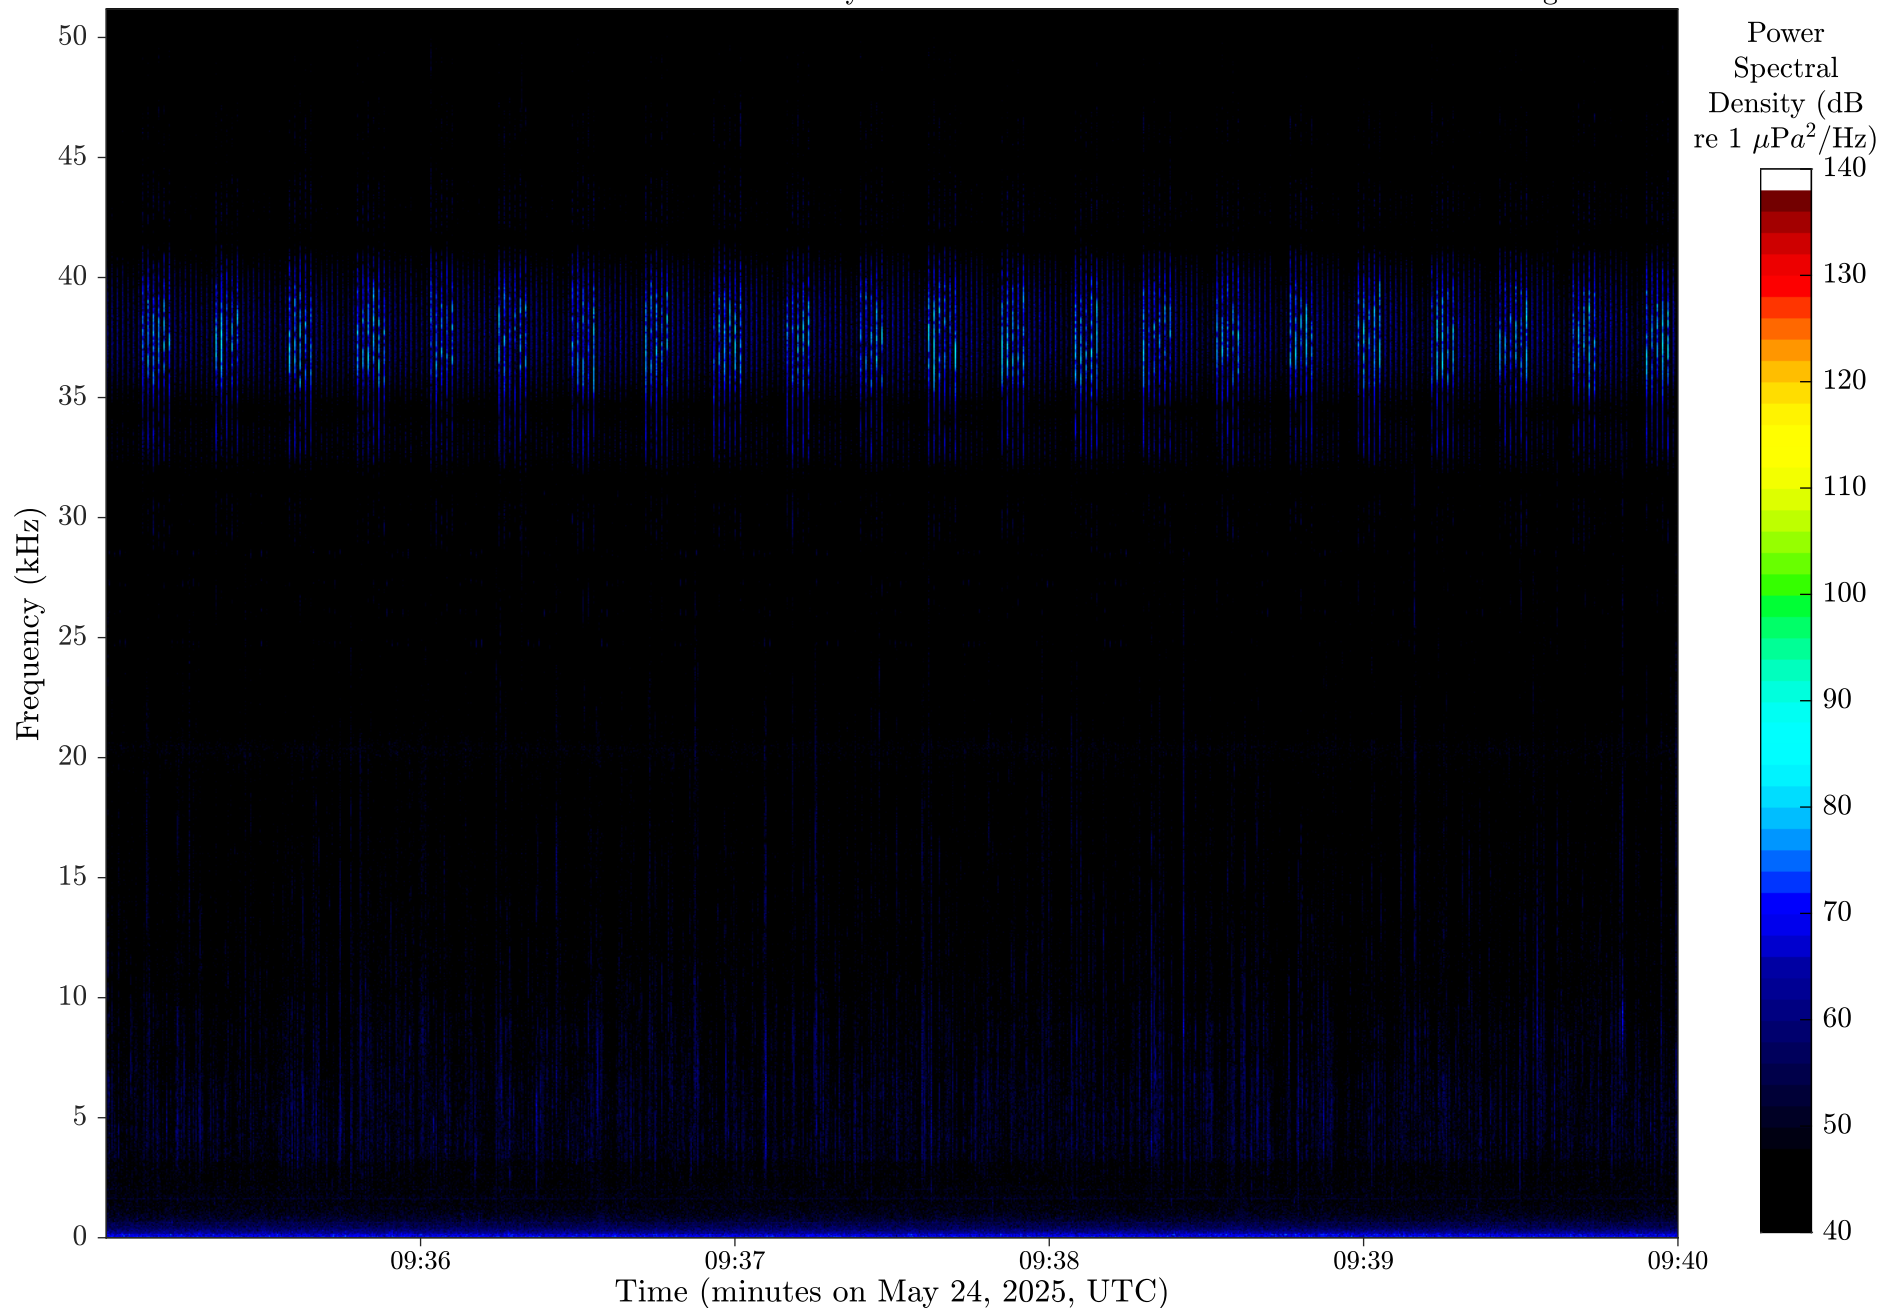


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:06 UTC

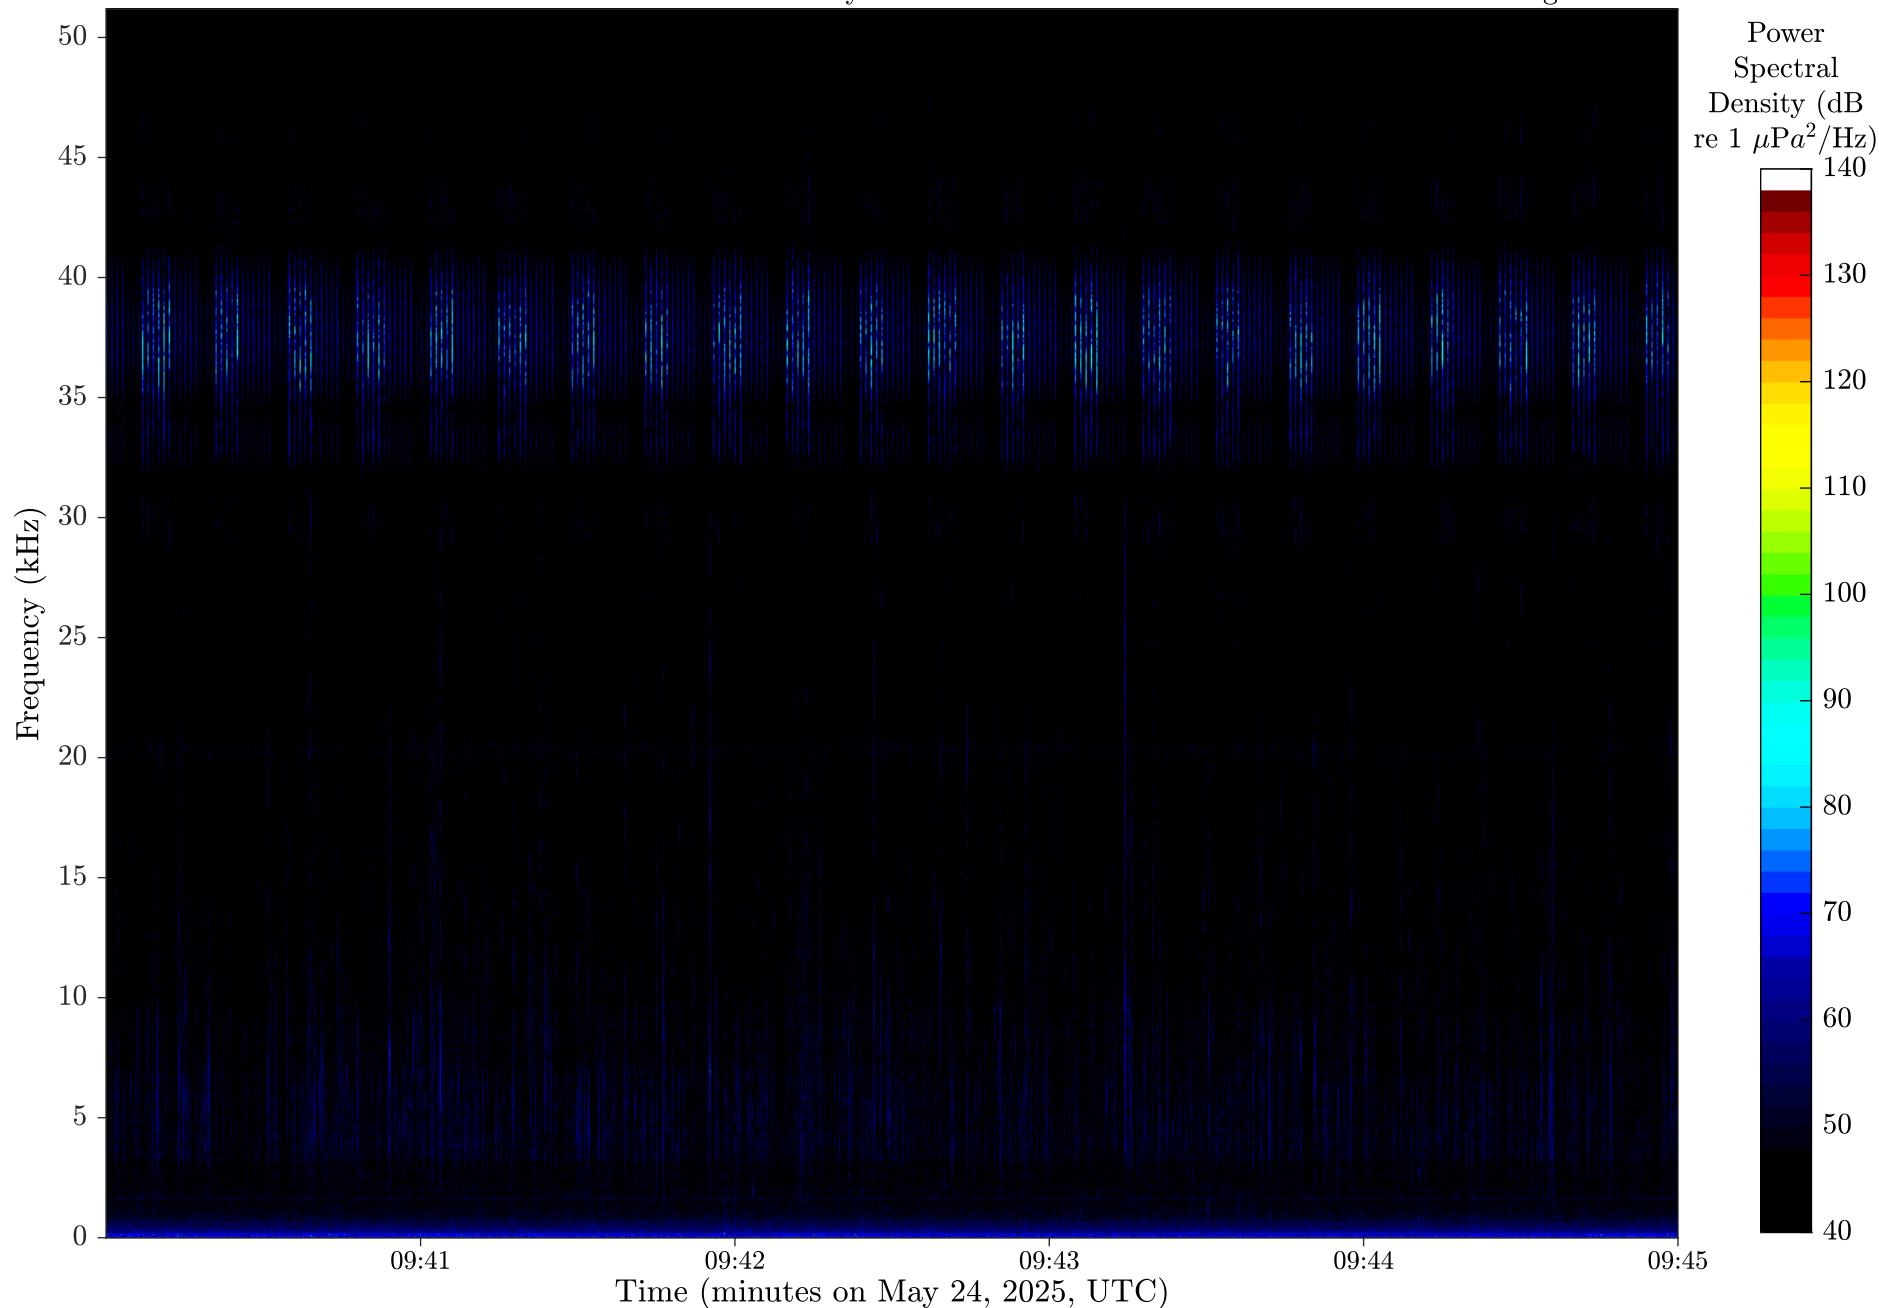


Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:14 UTC

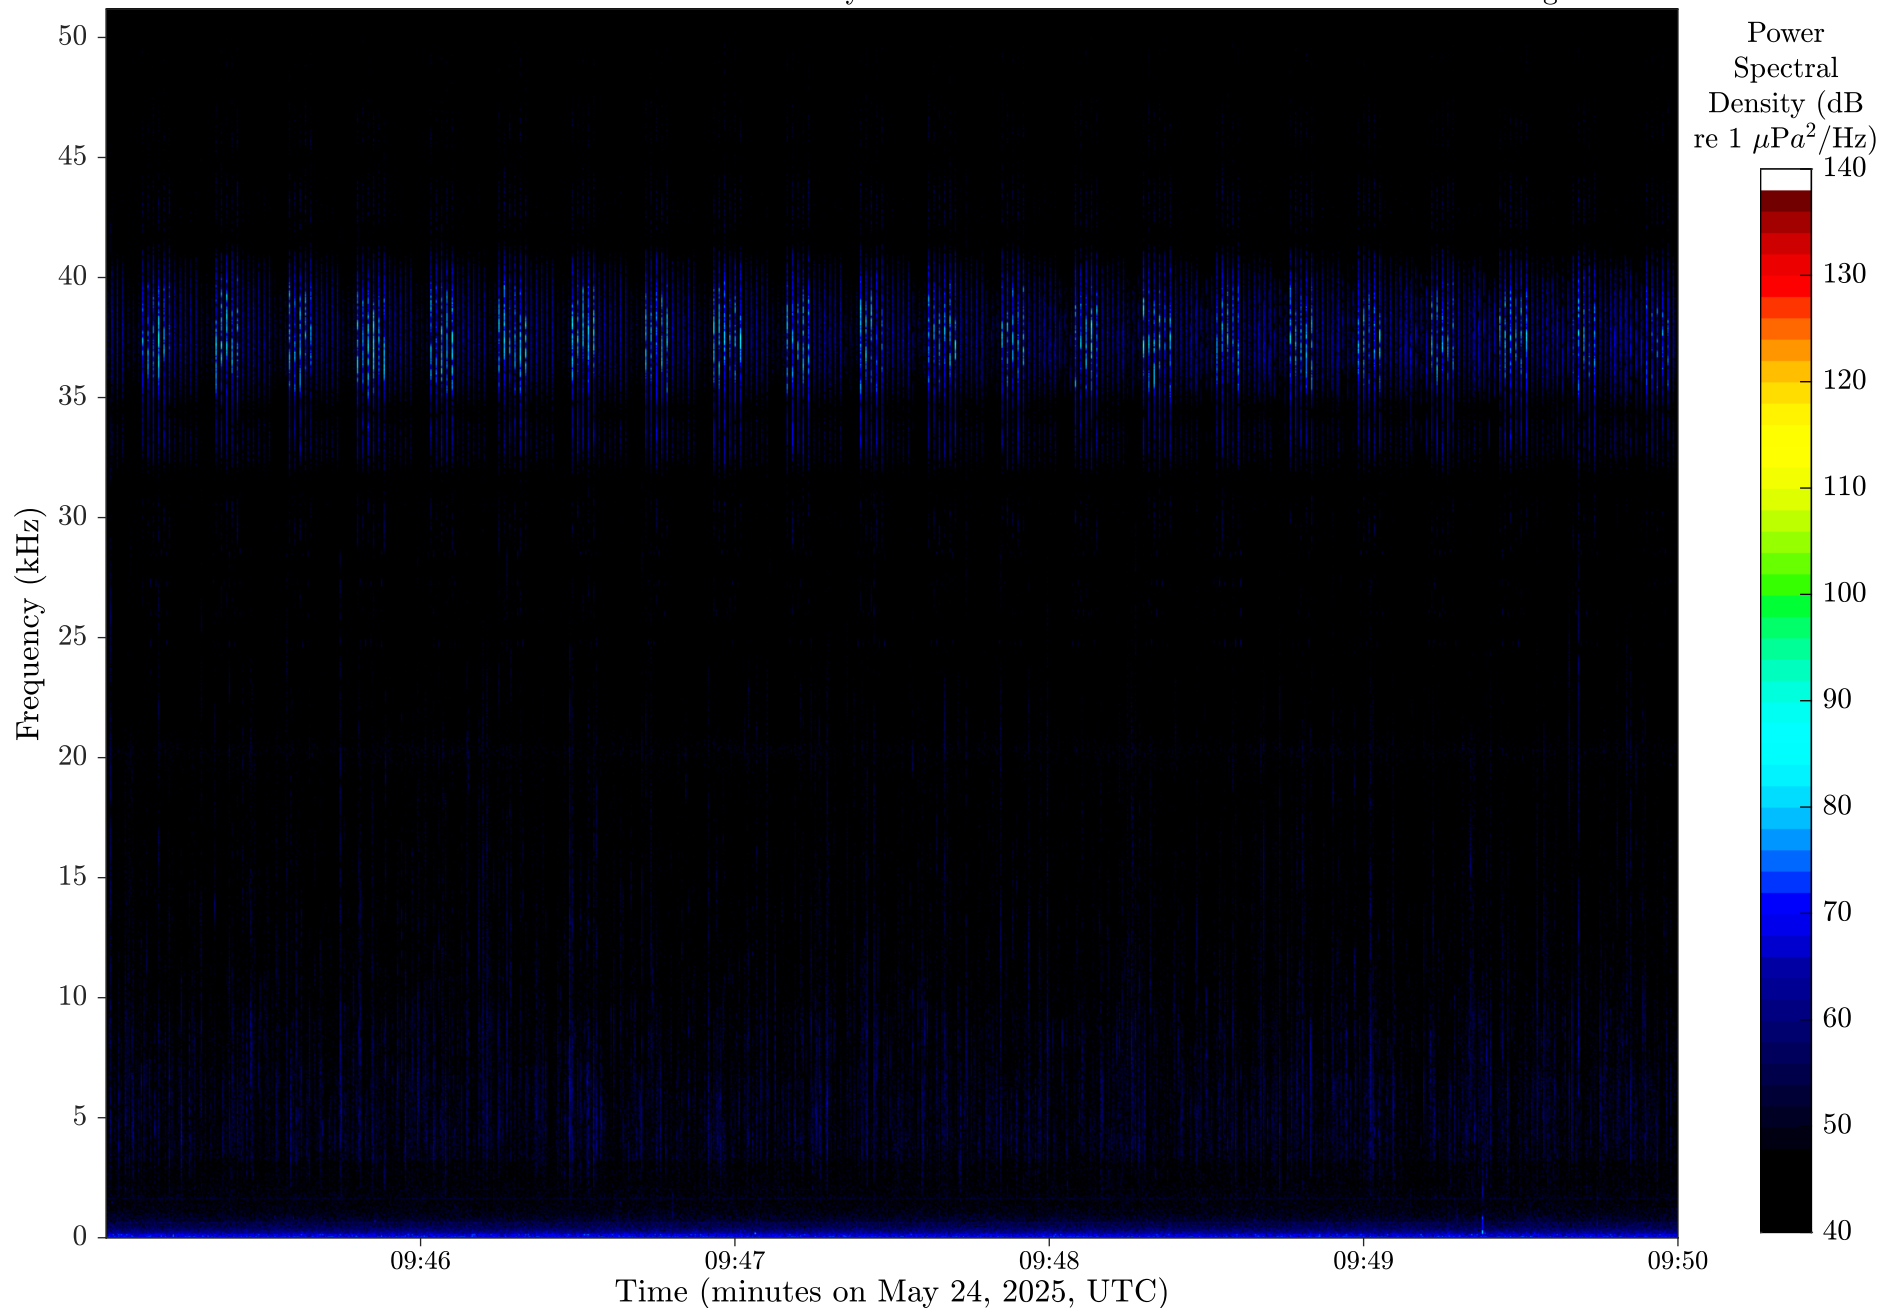


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:22 UTC

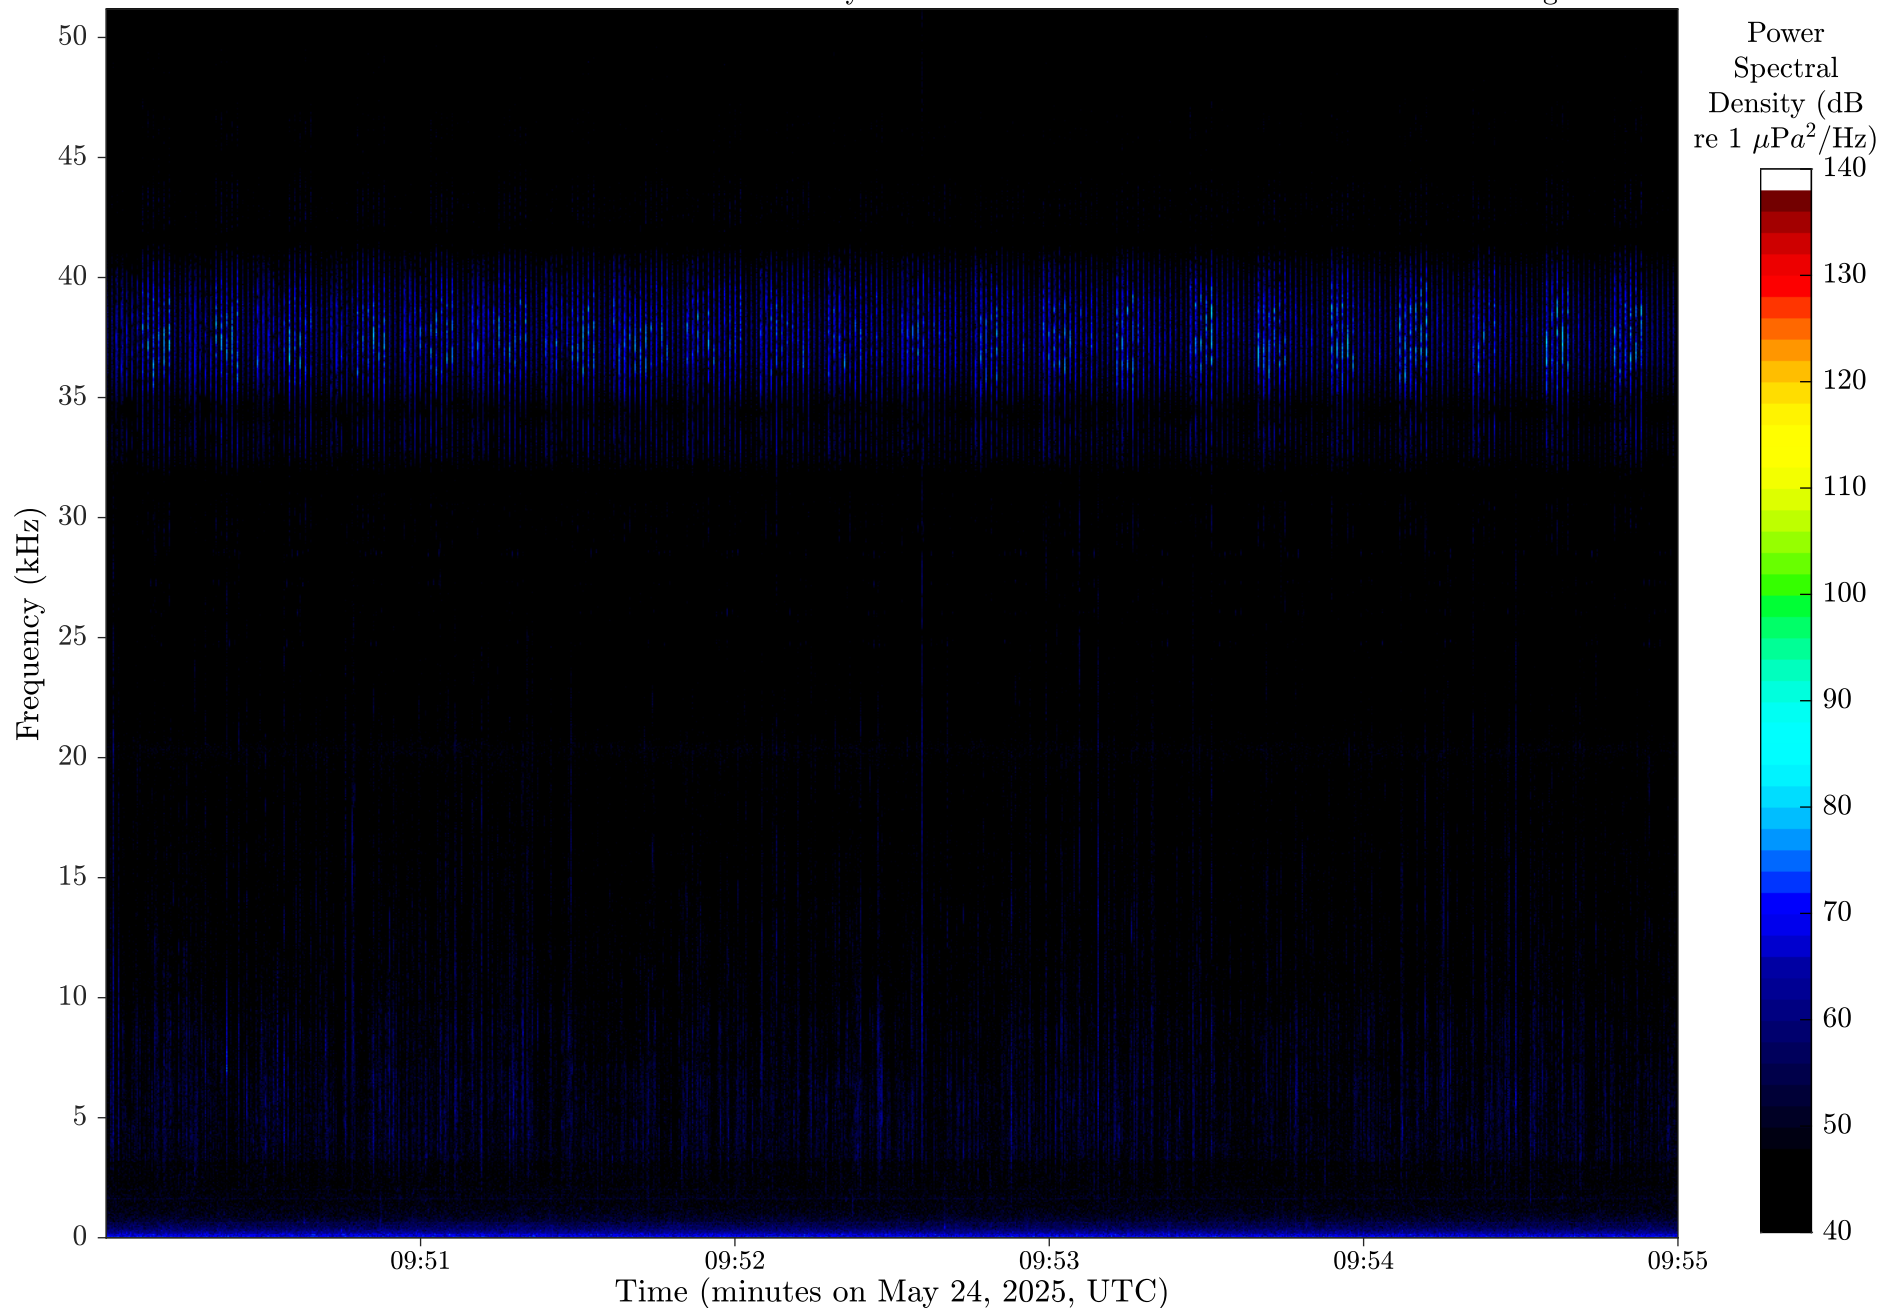


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:31 UTC

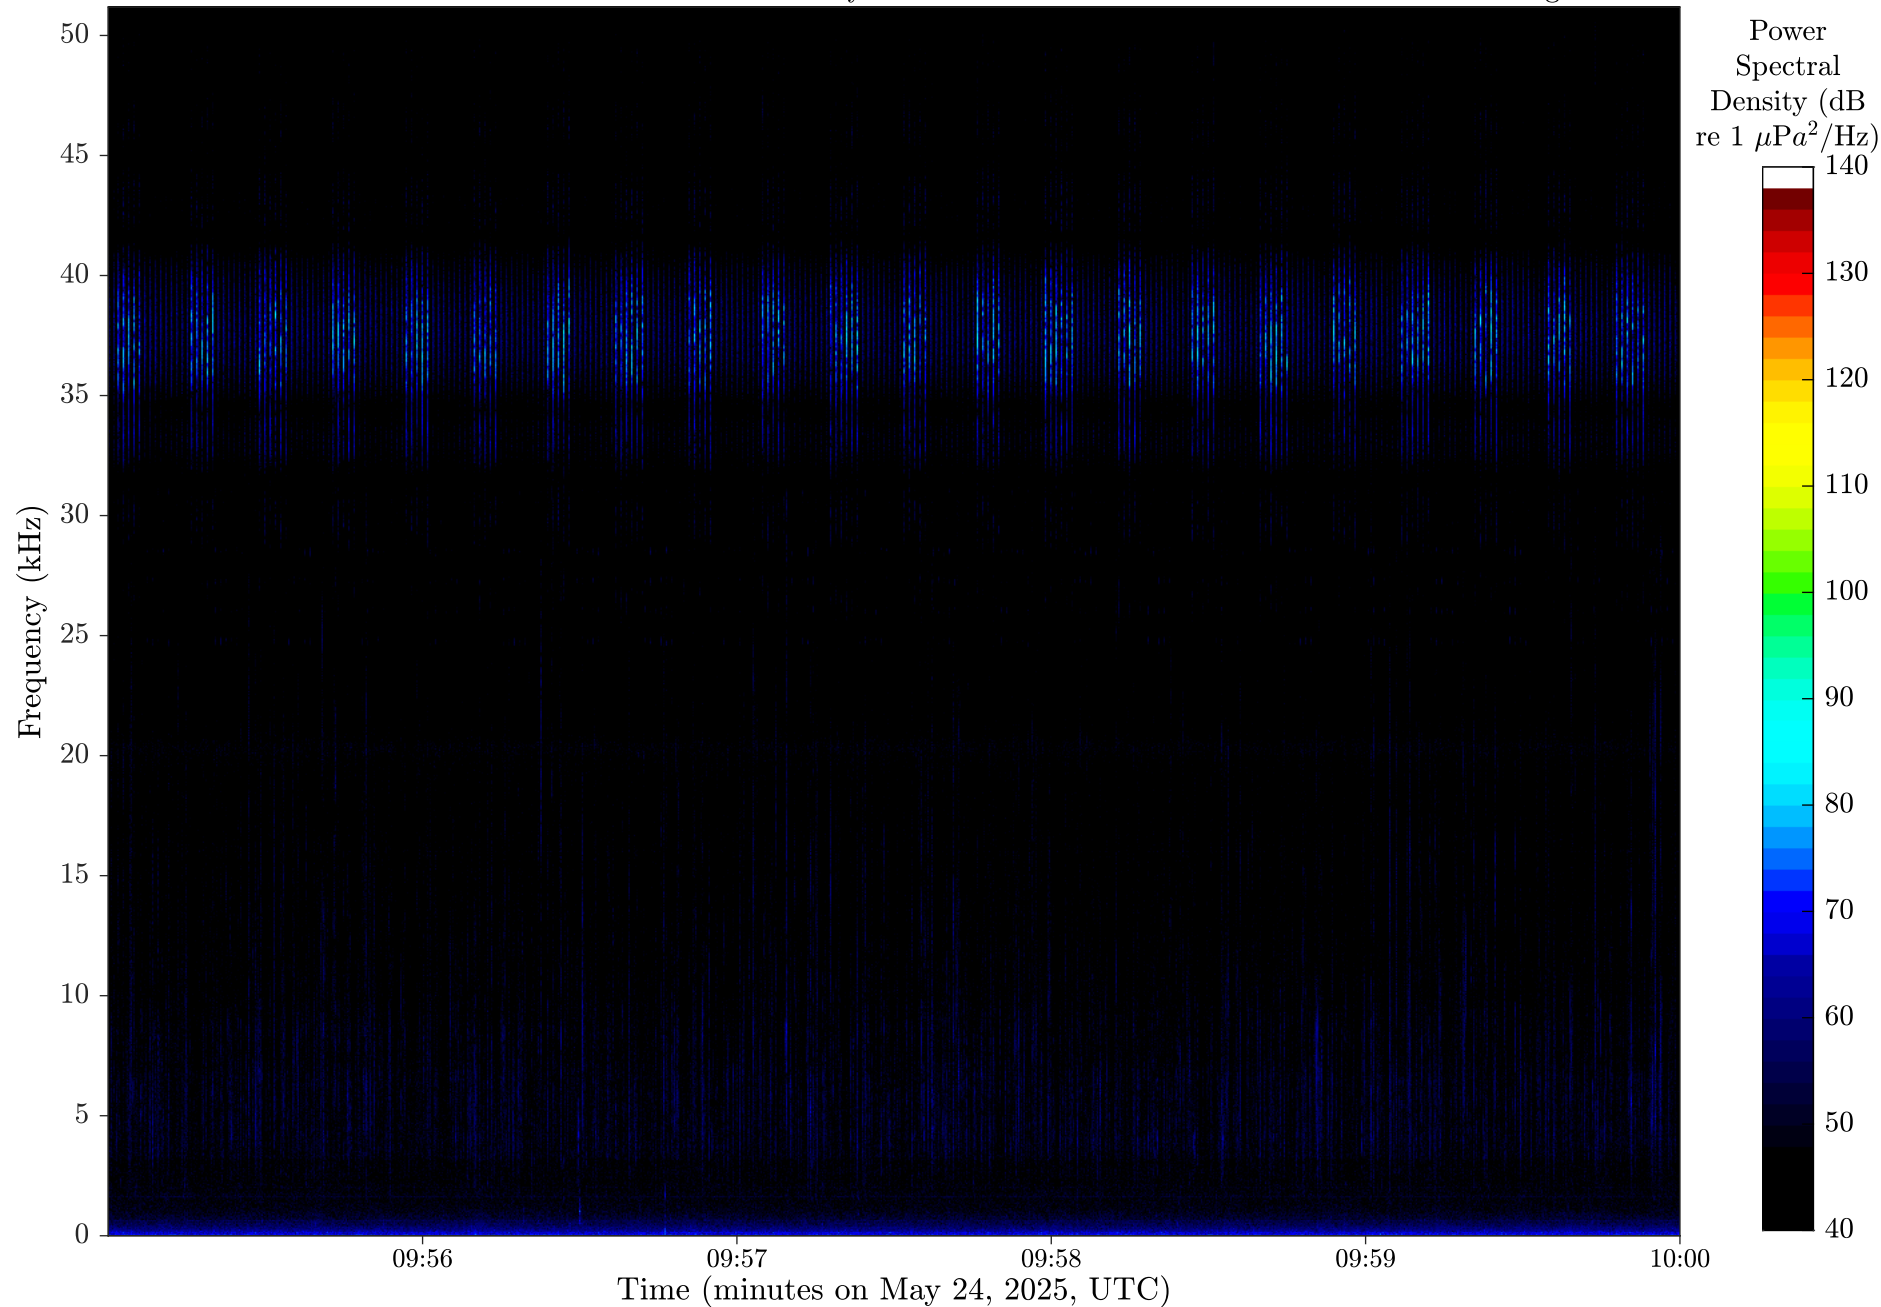


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:39 UTC

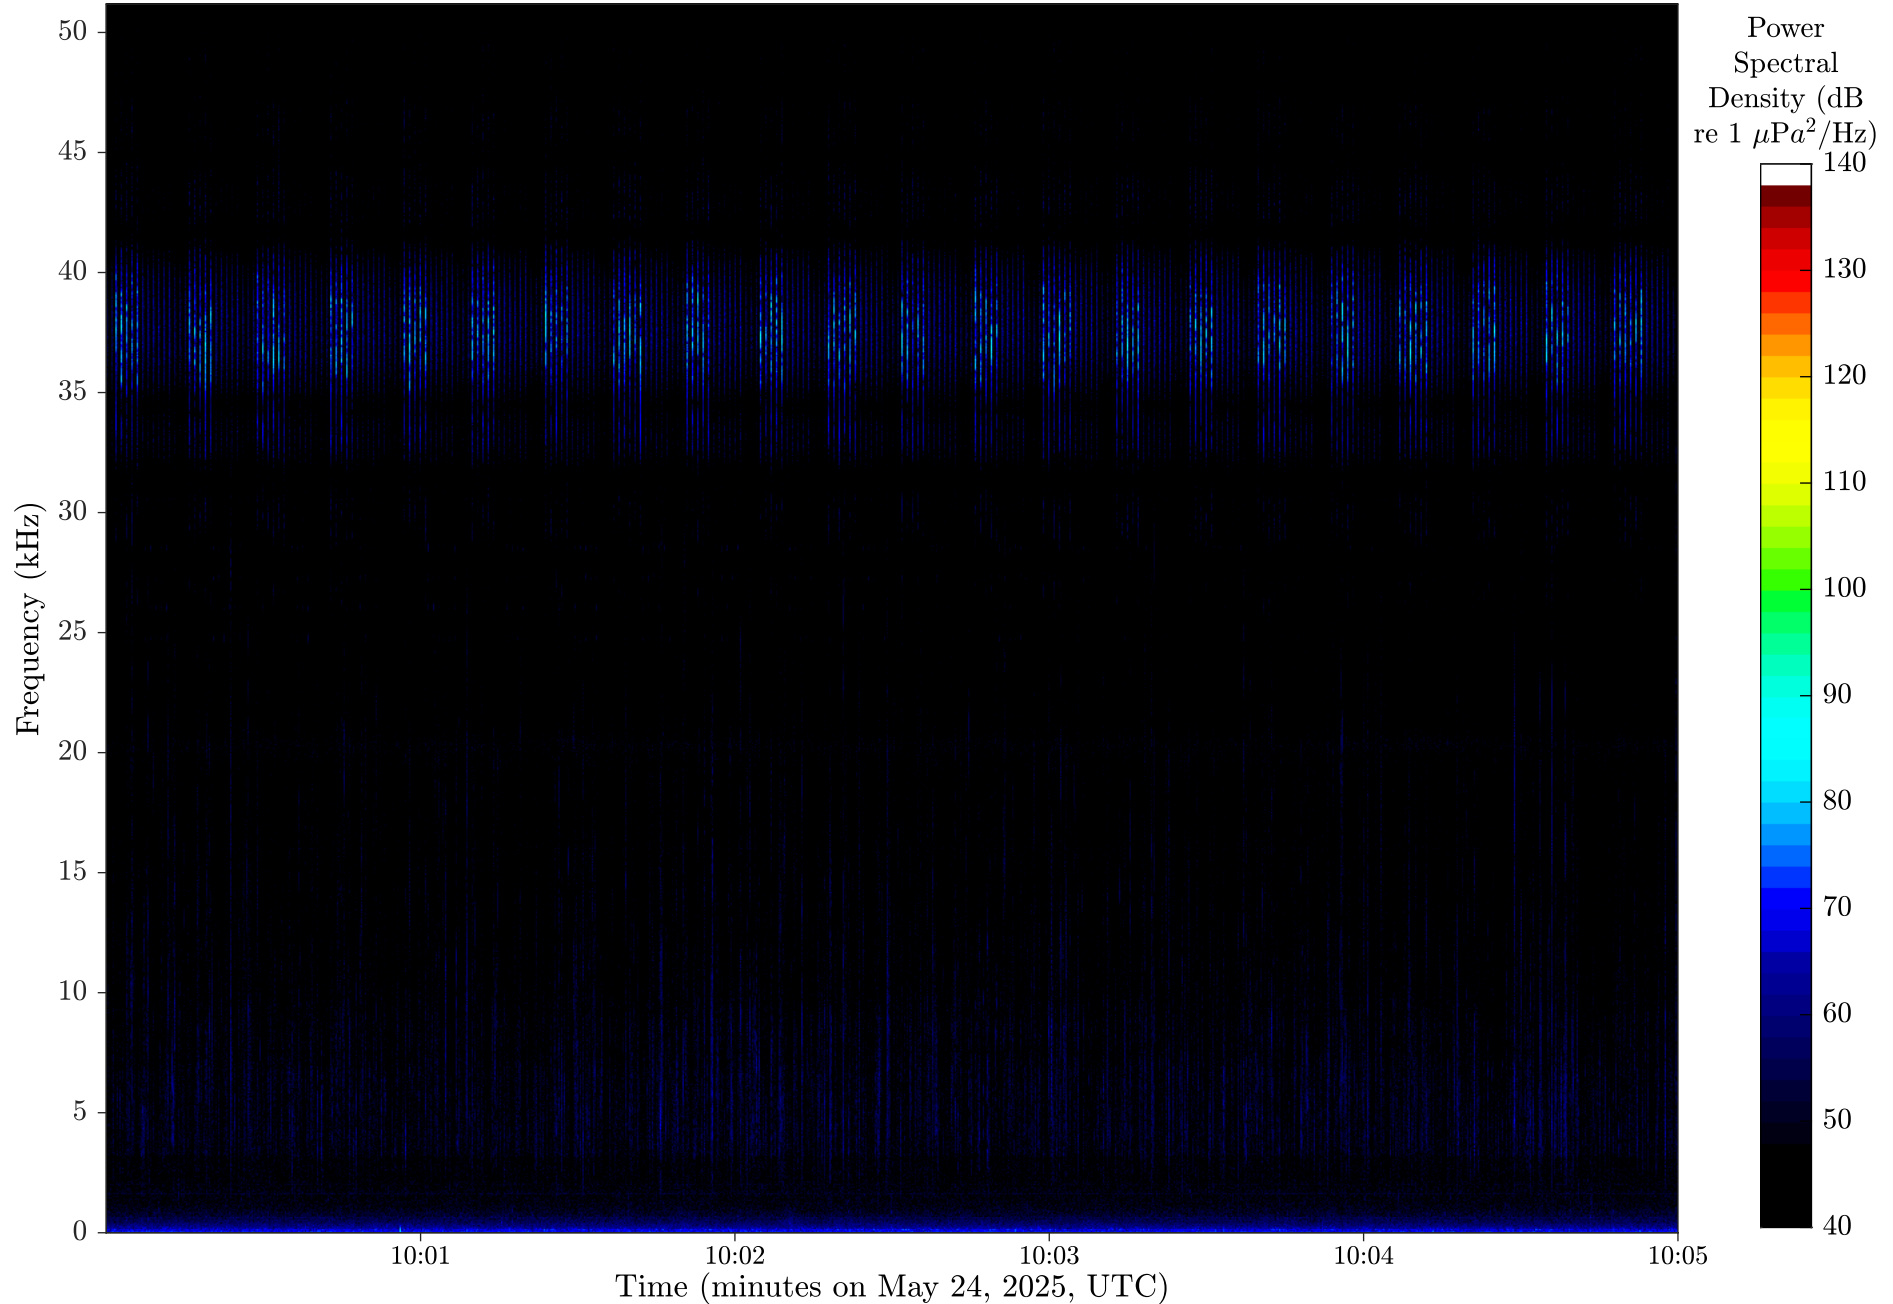


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:47 UTC

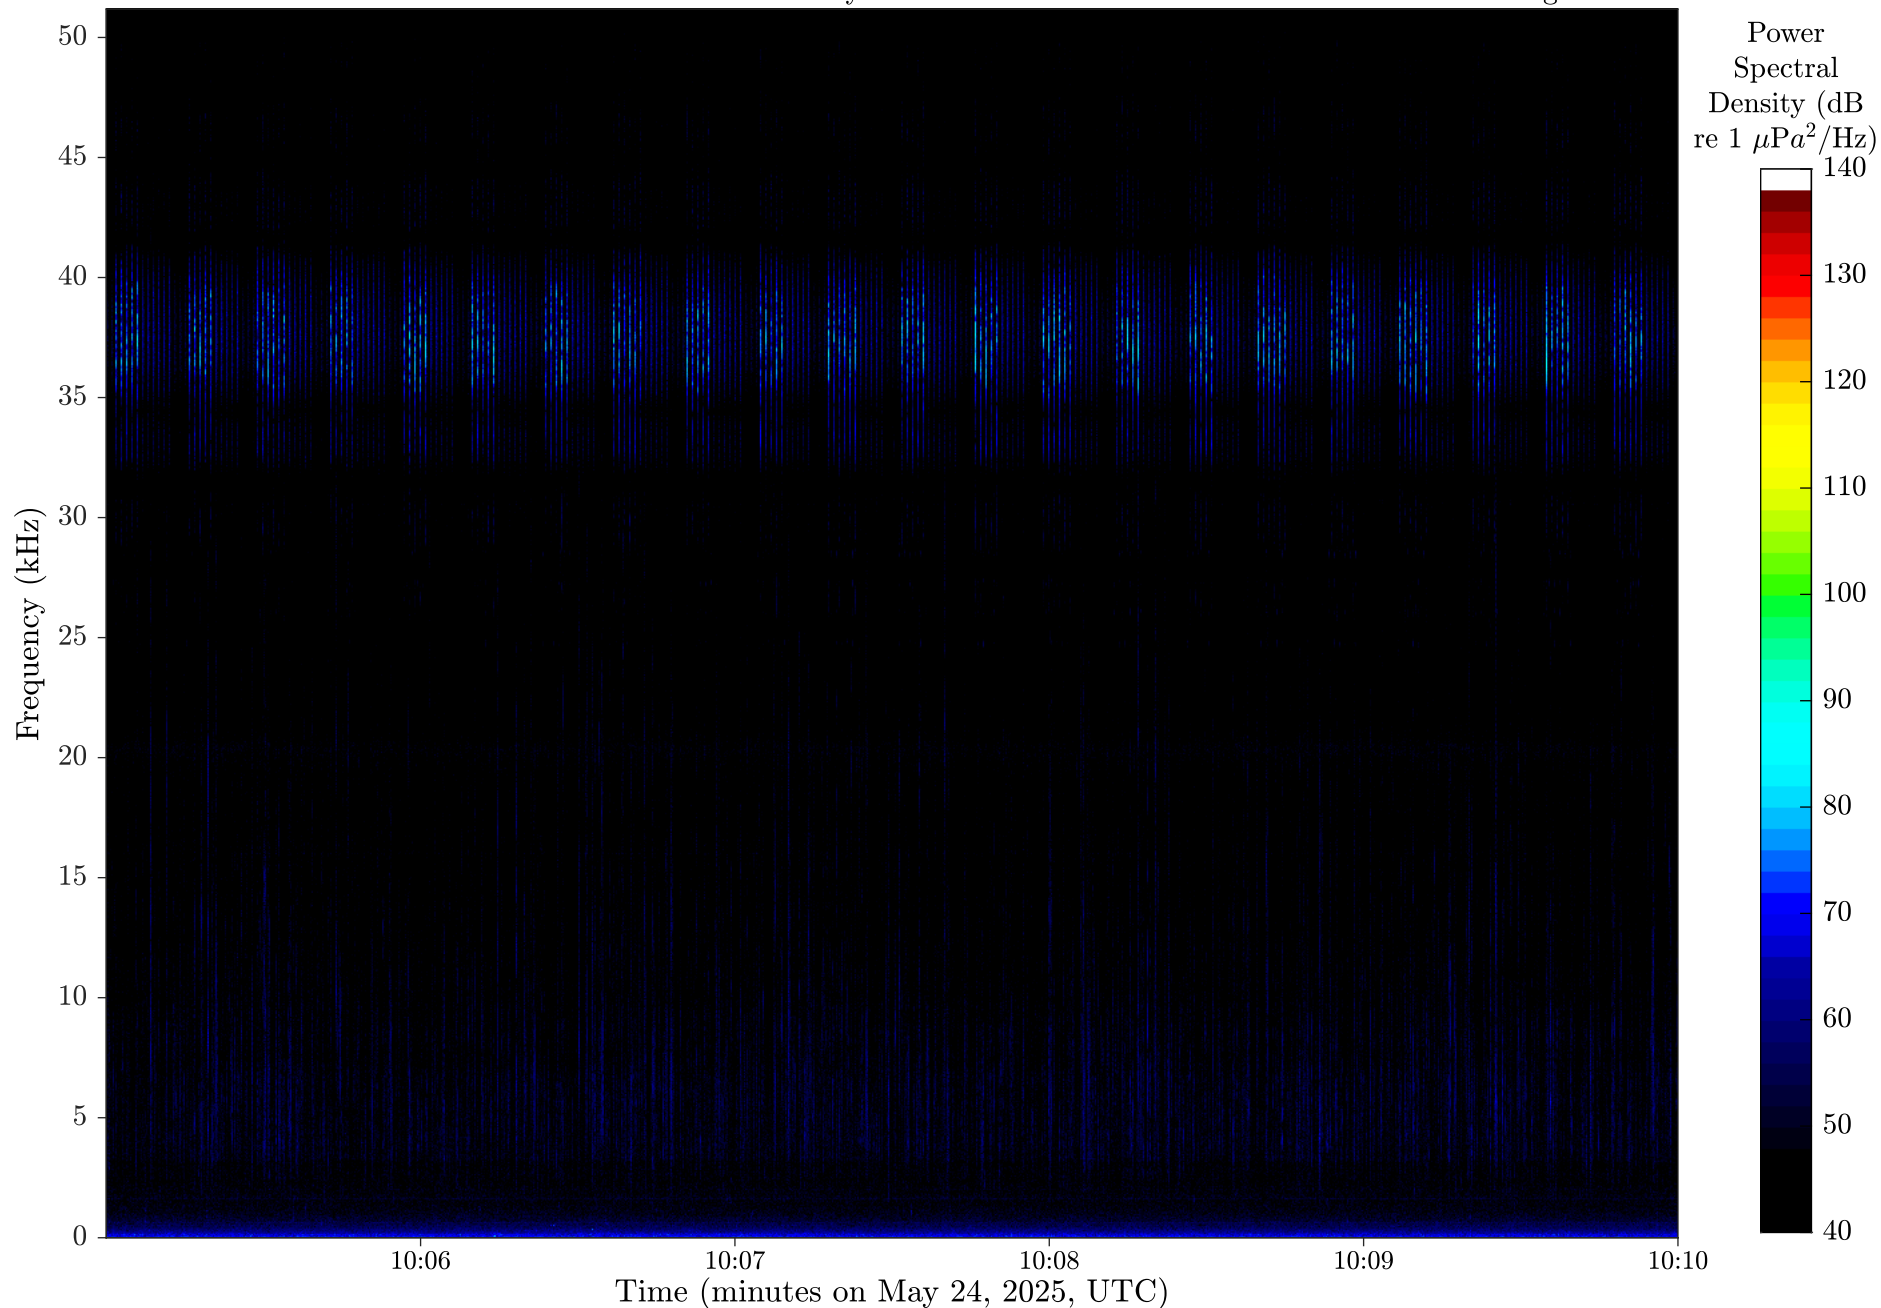


Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:23:56 UTC

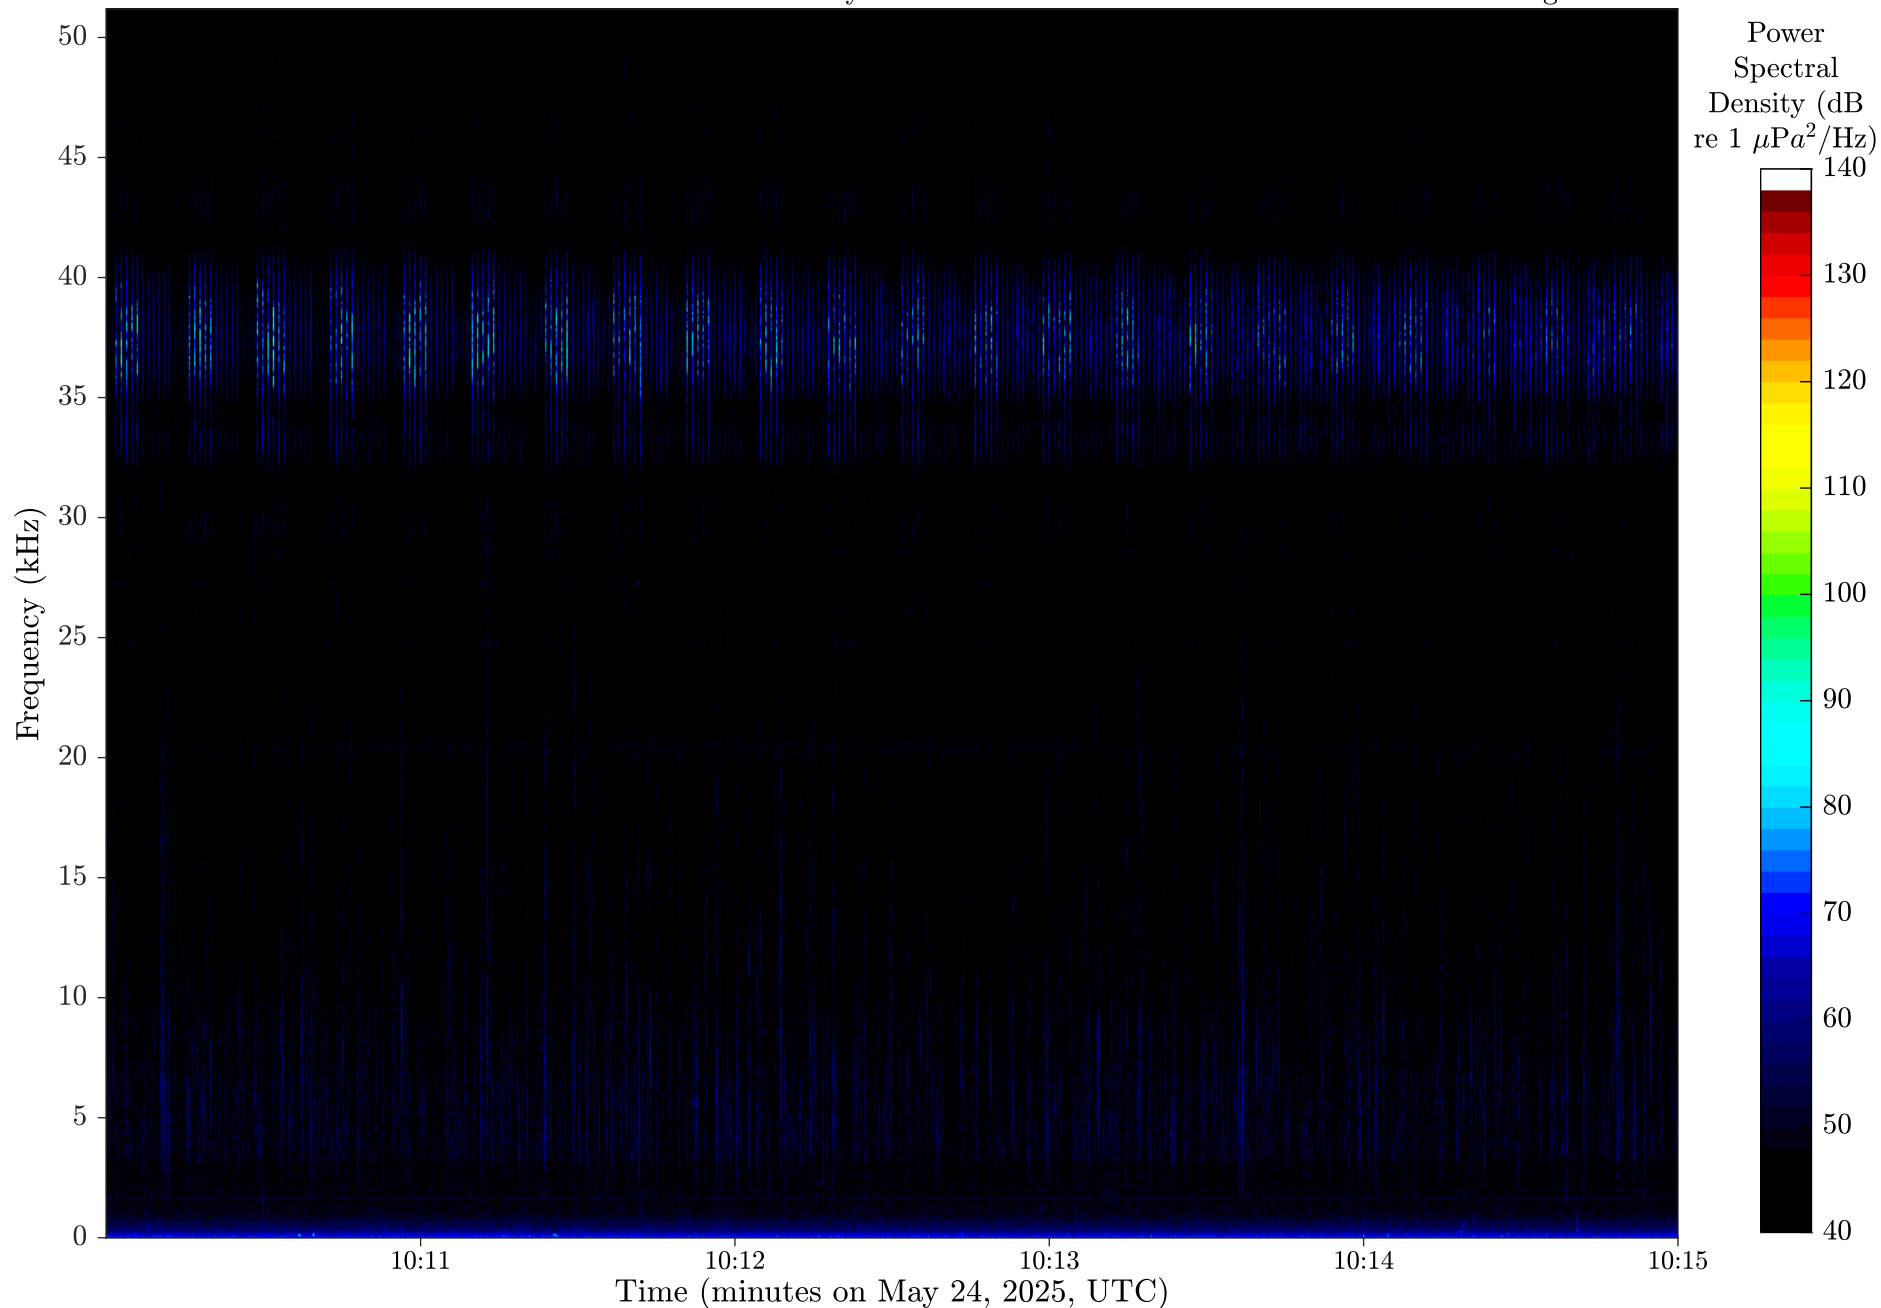


Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:24:06 UTC

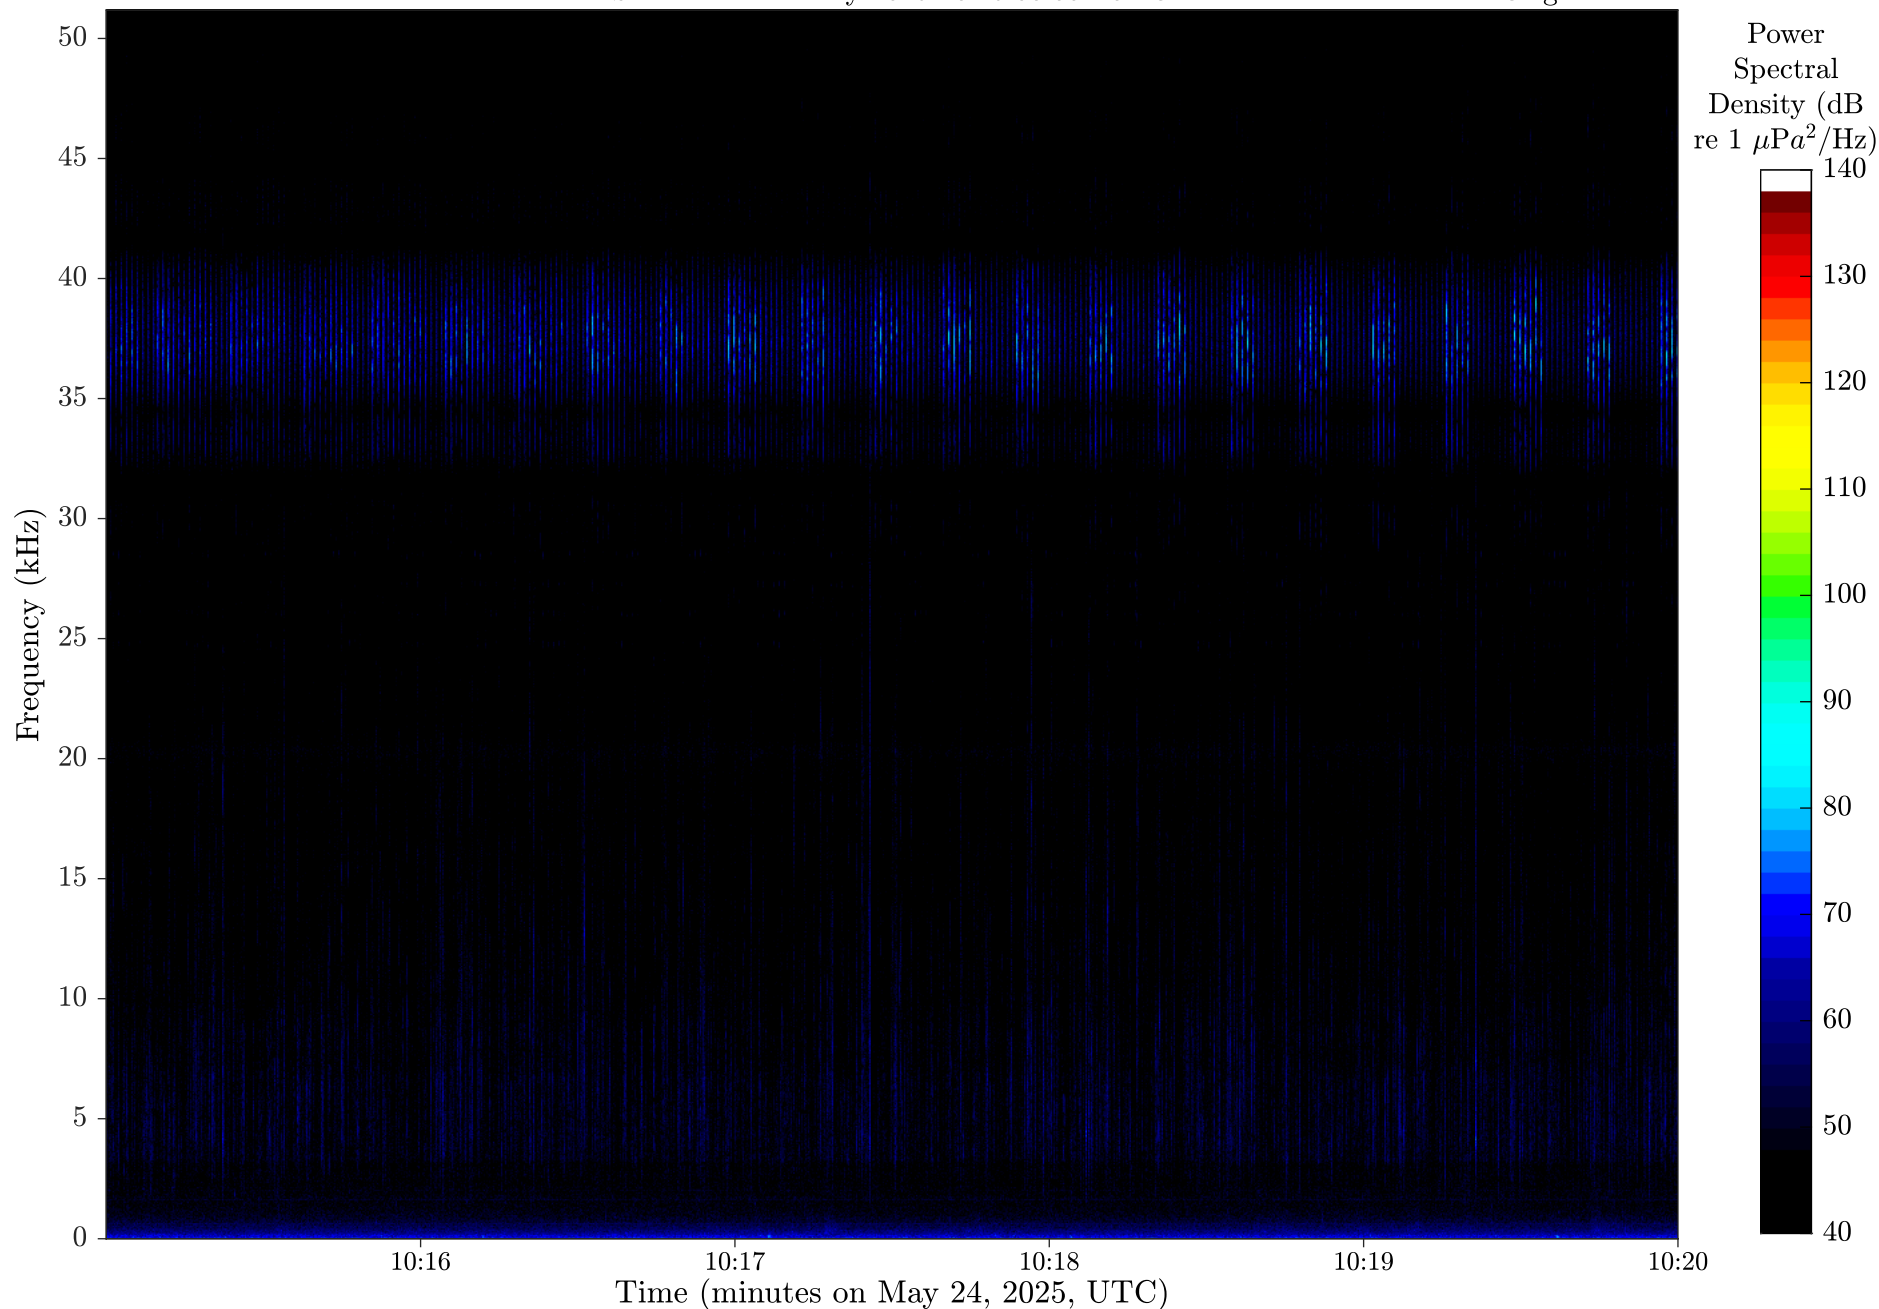


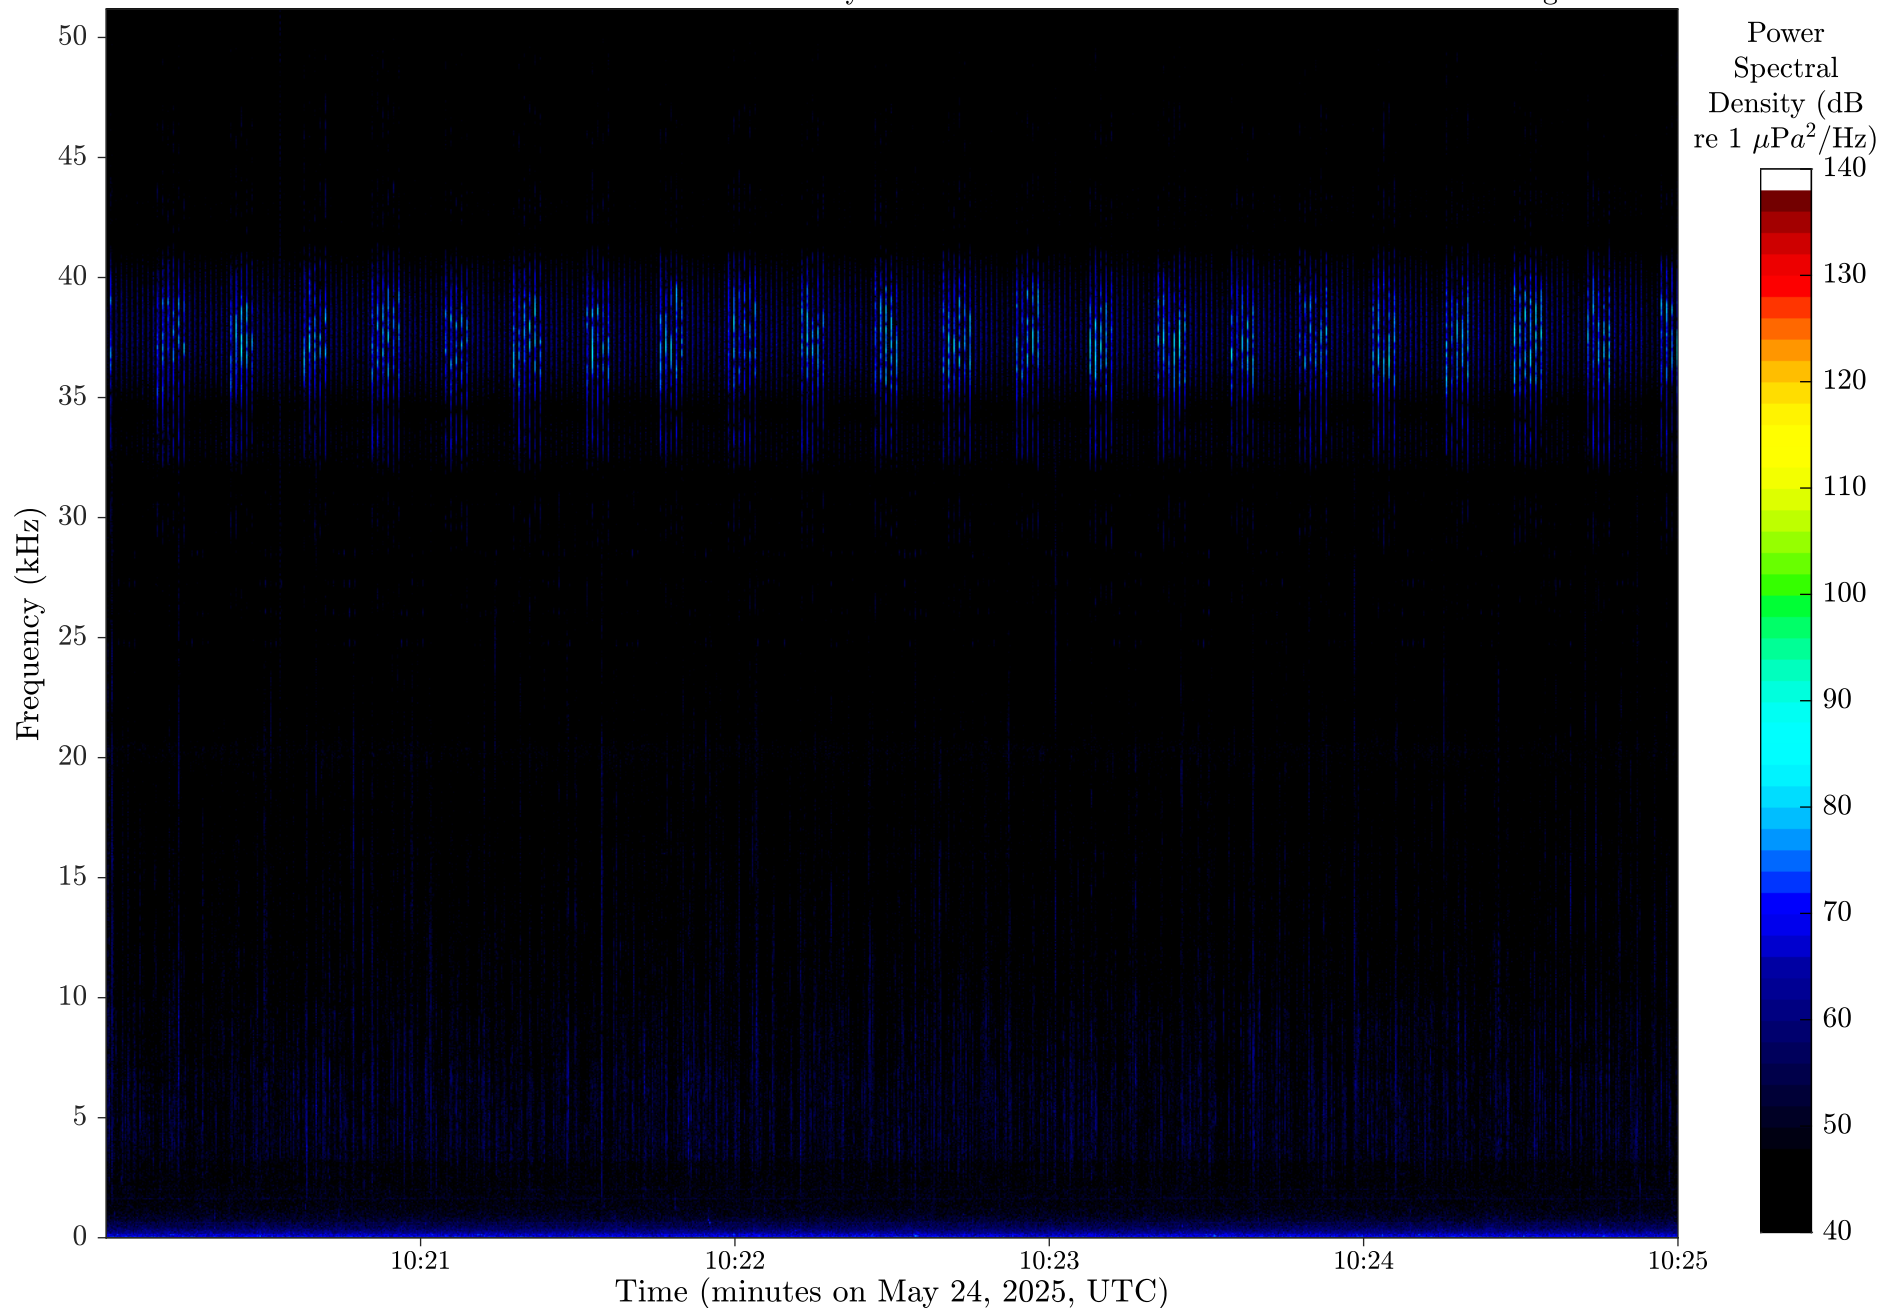


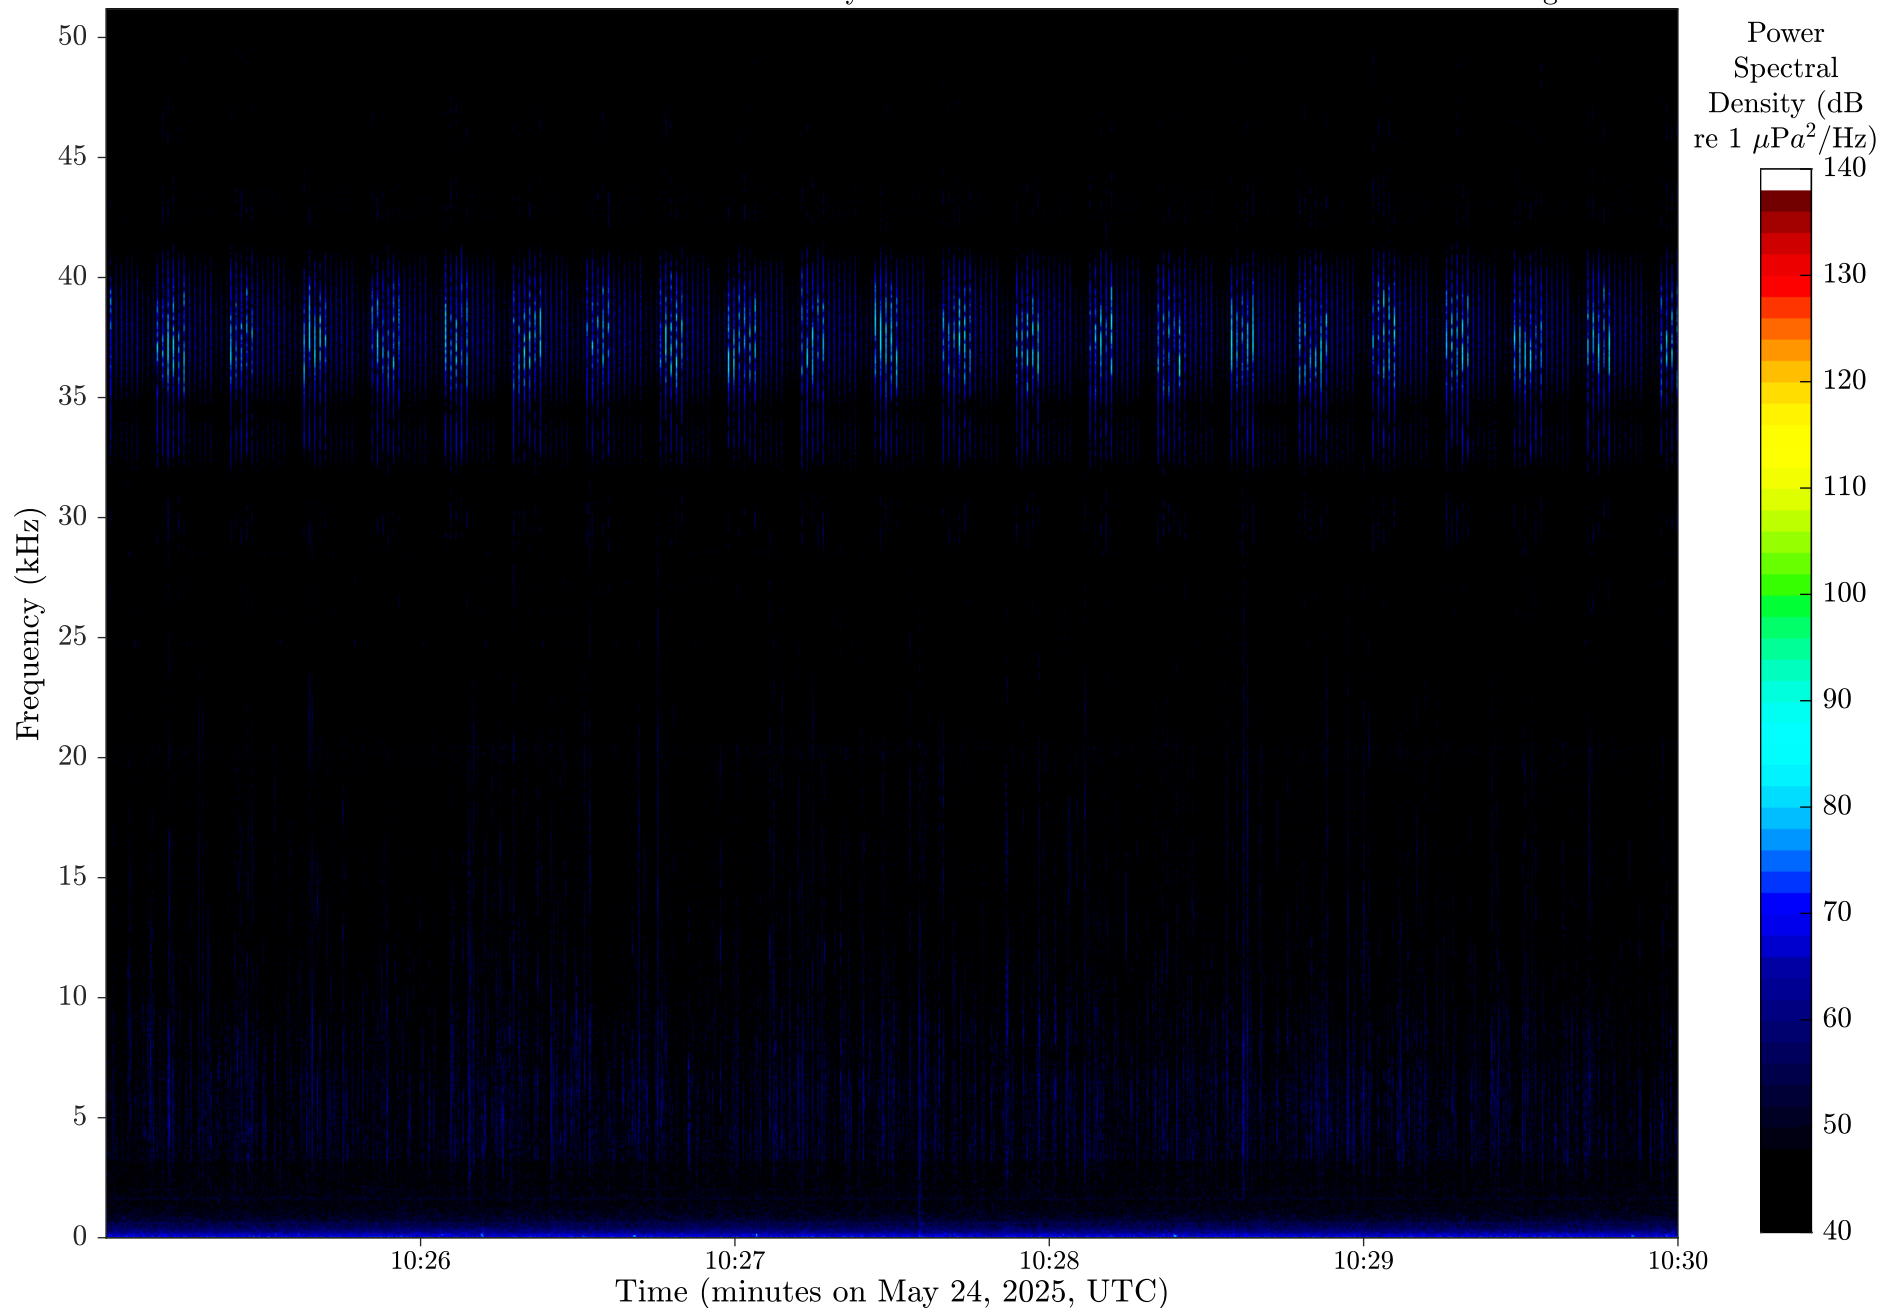

Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:24:31 UTC

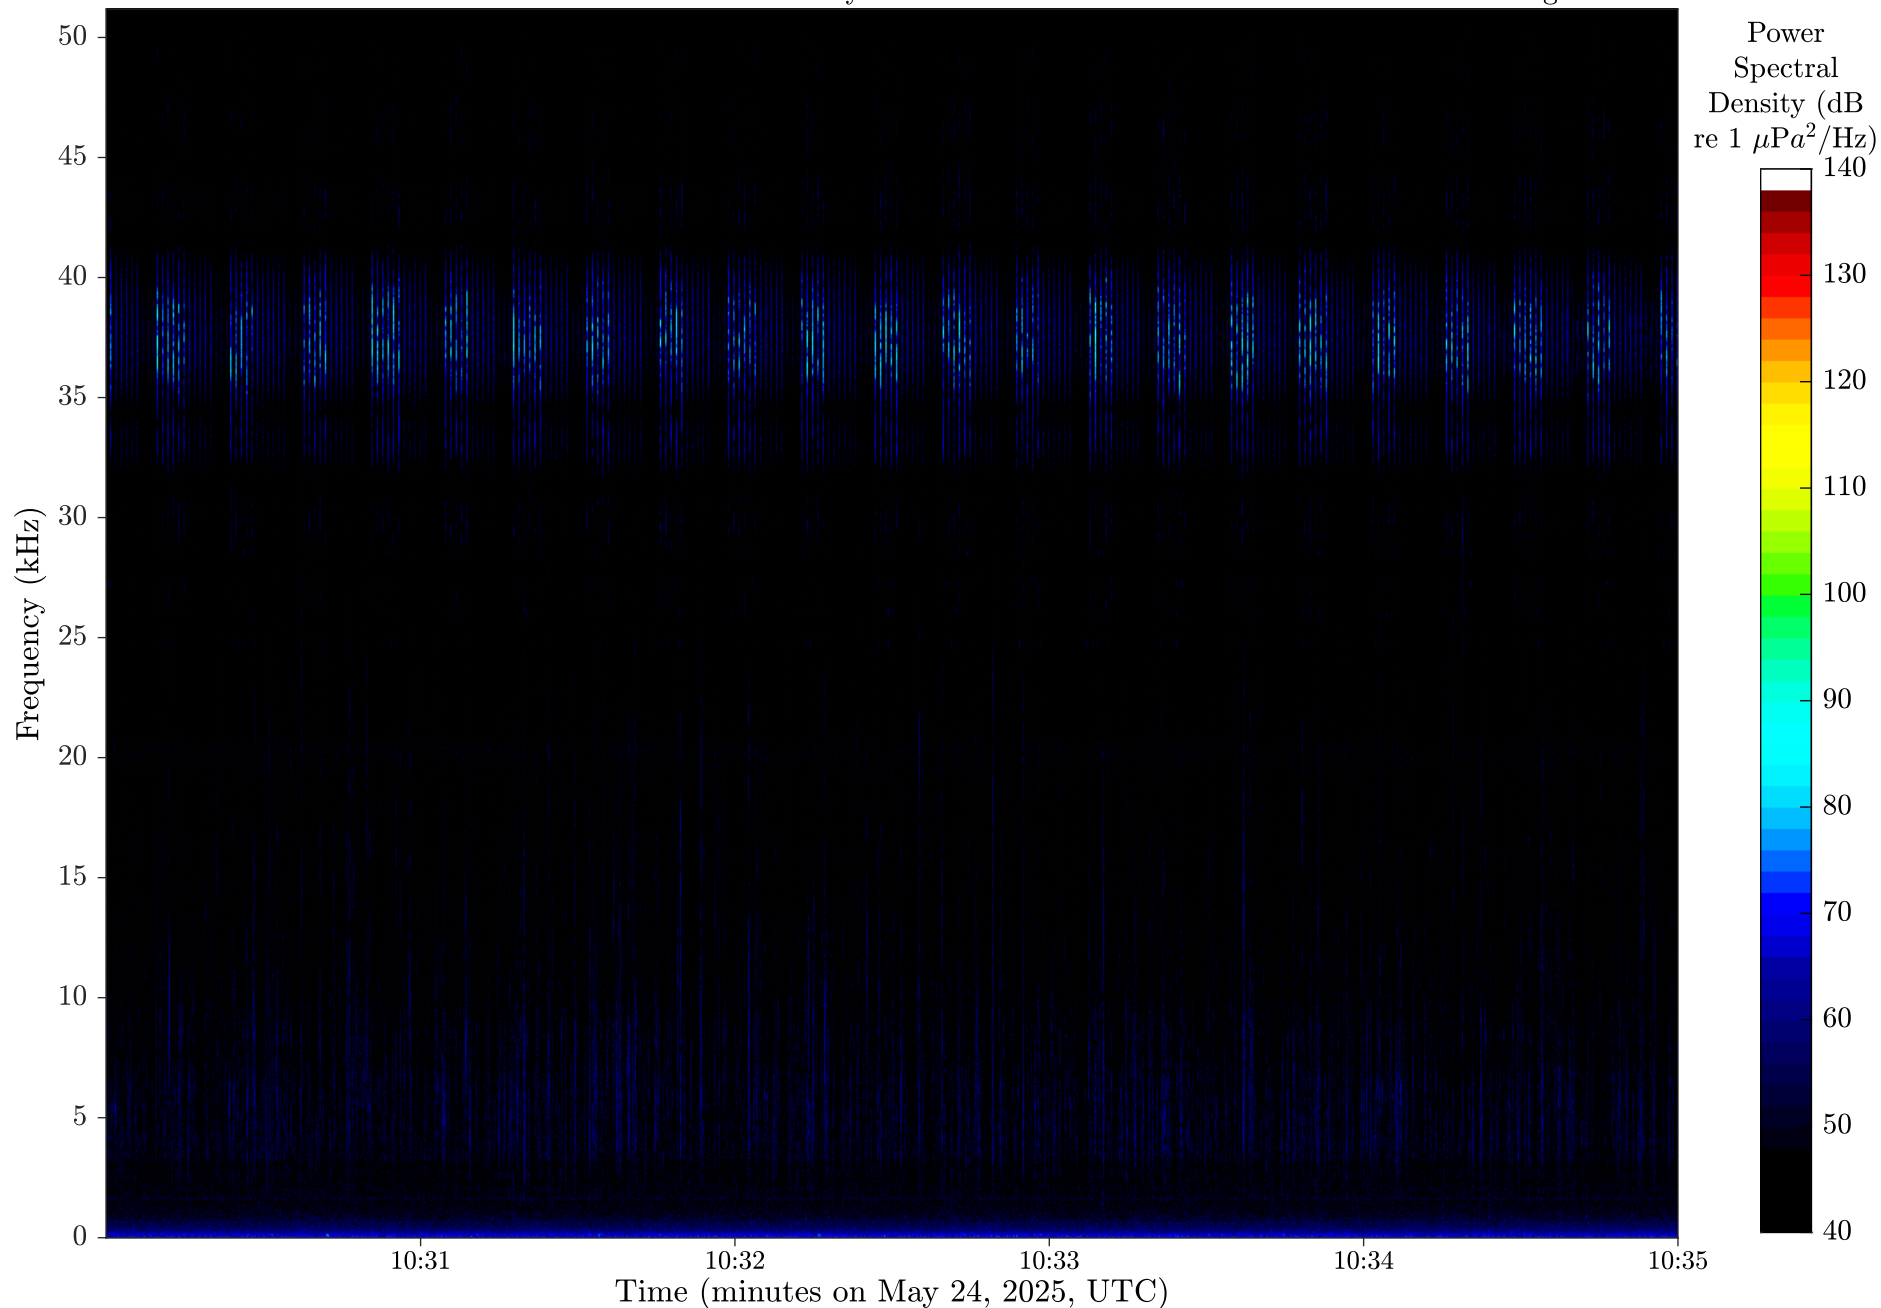

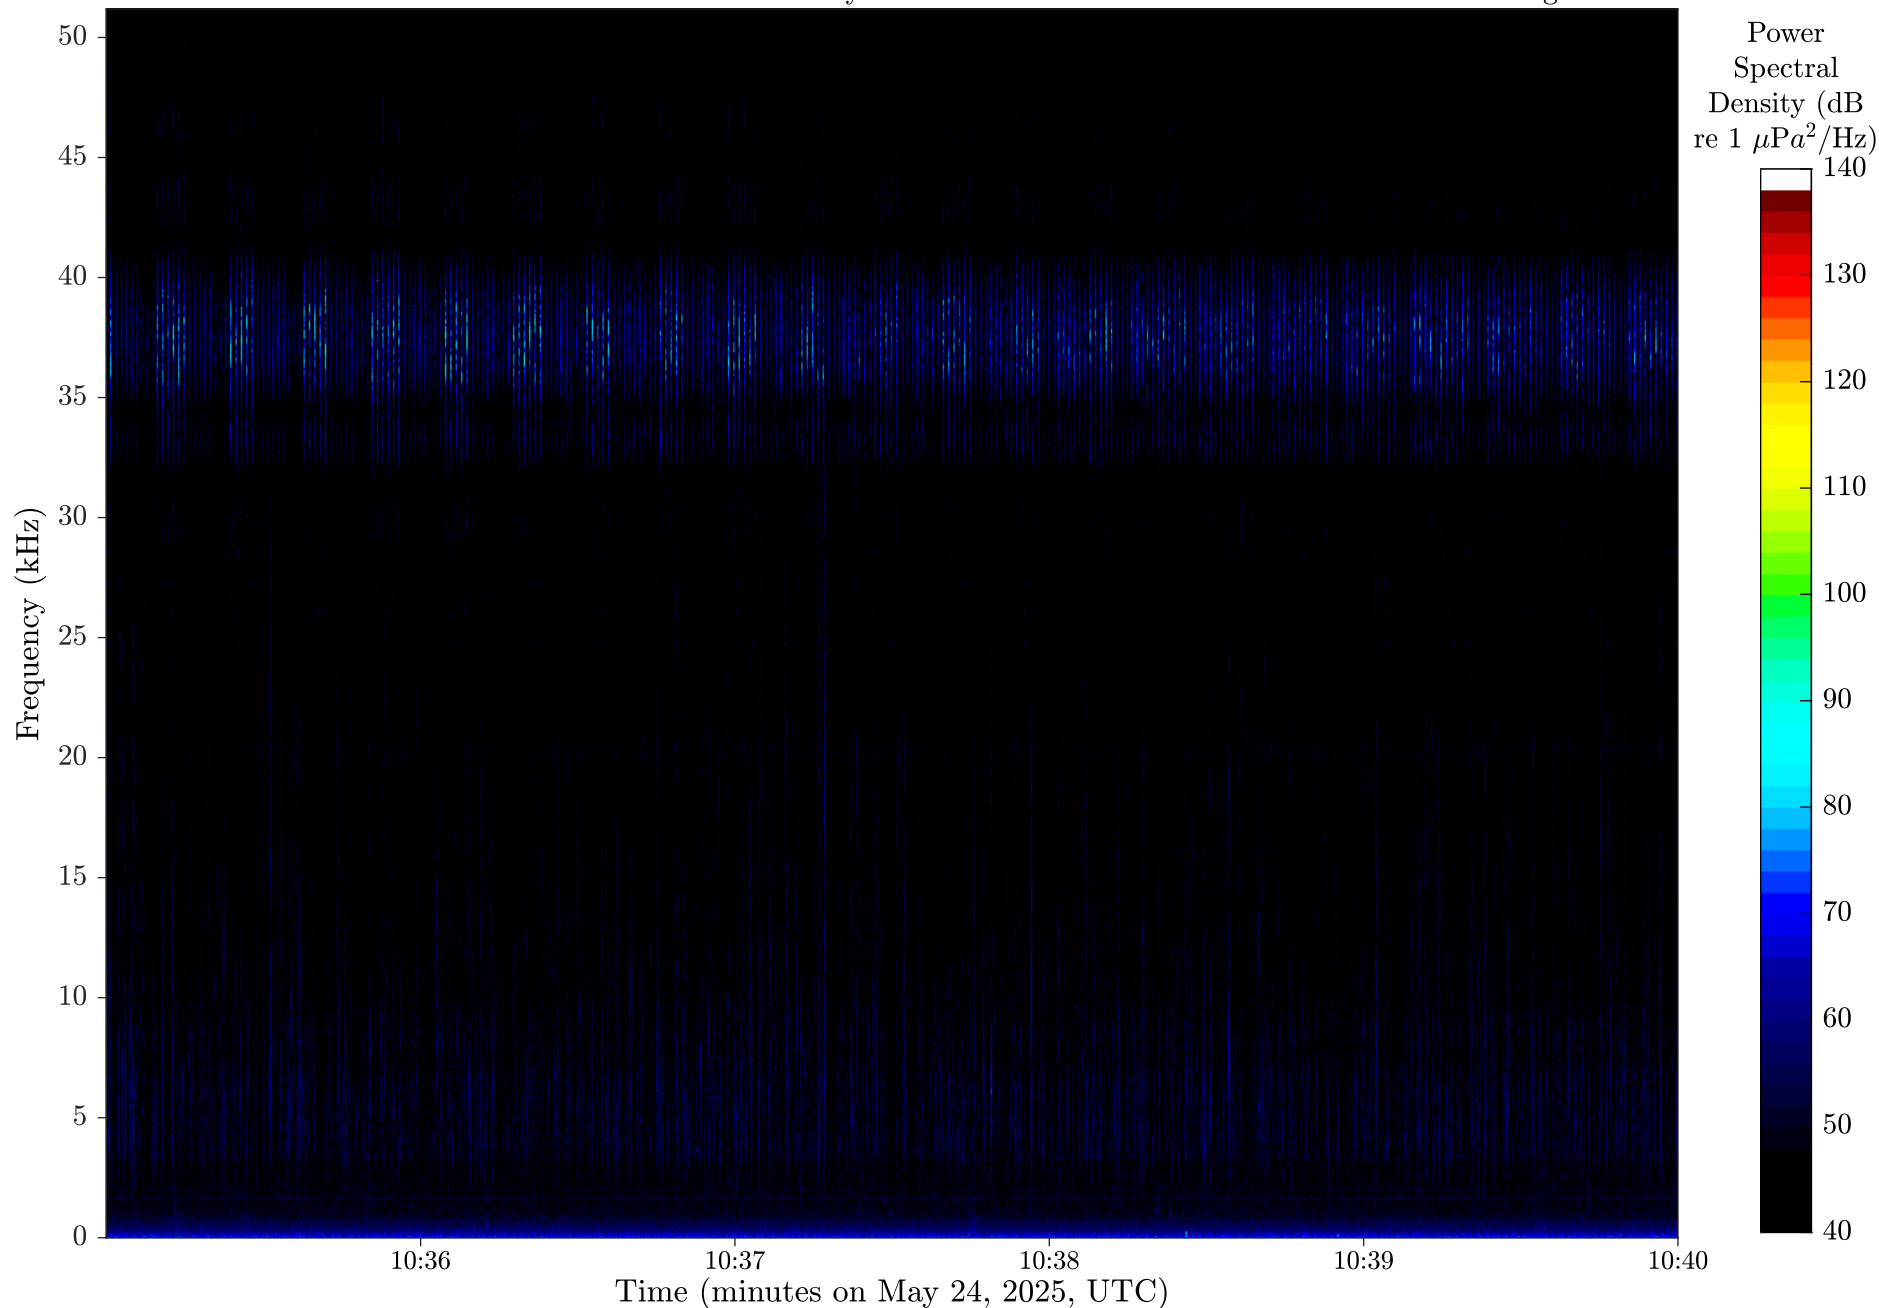


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:24:49 UTC

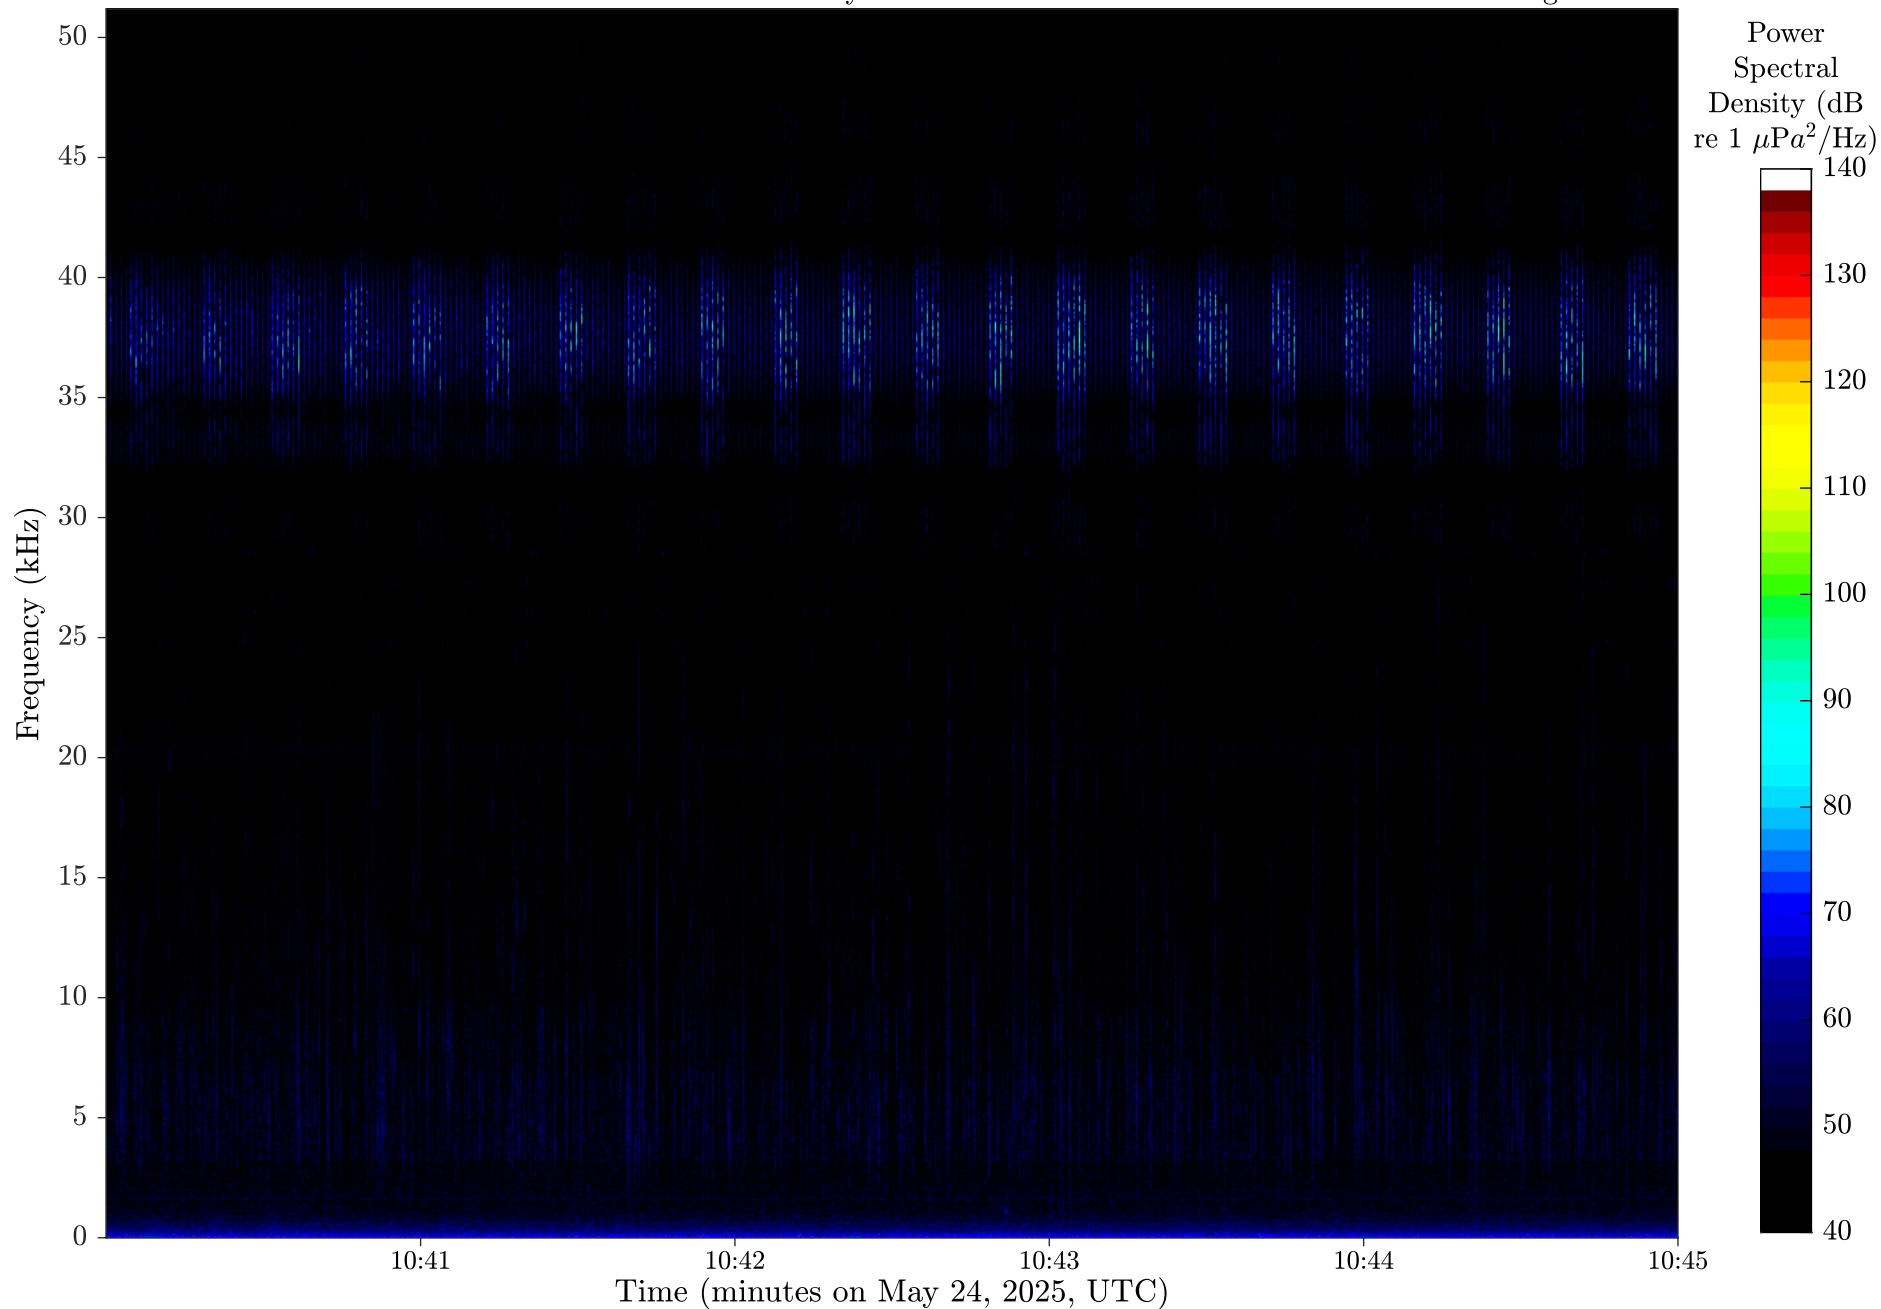


Comments: 33.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:24:57 UTC

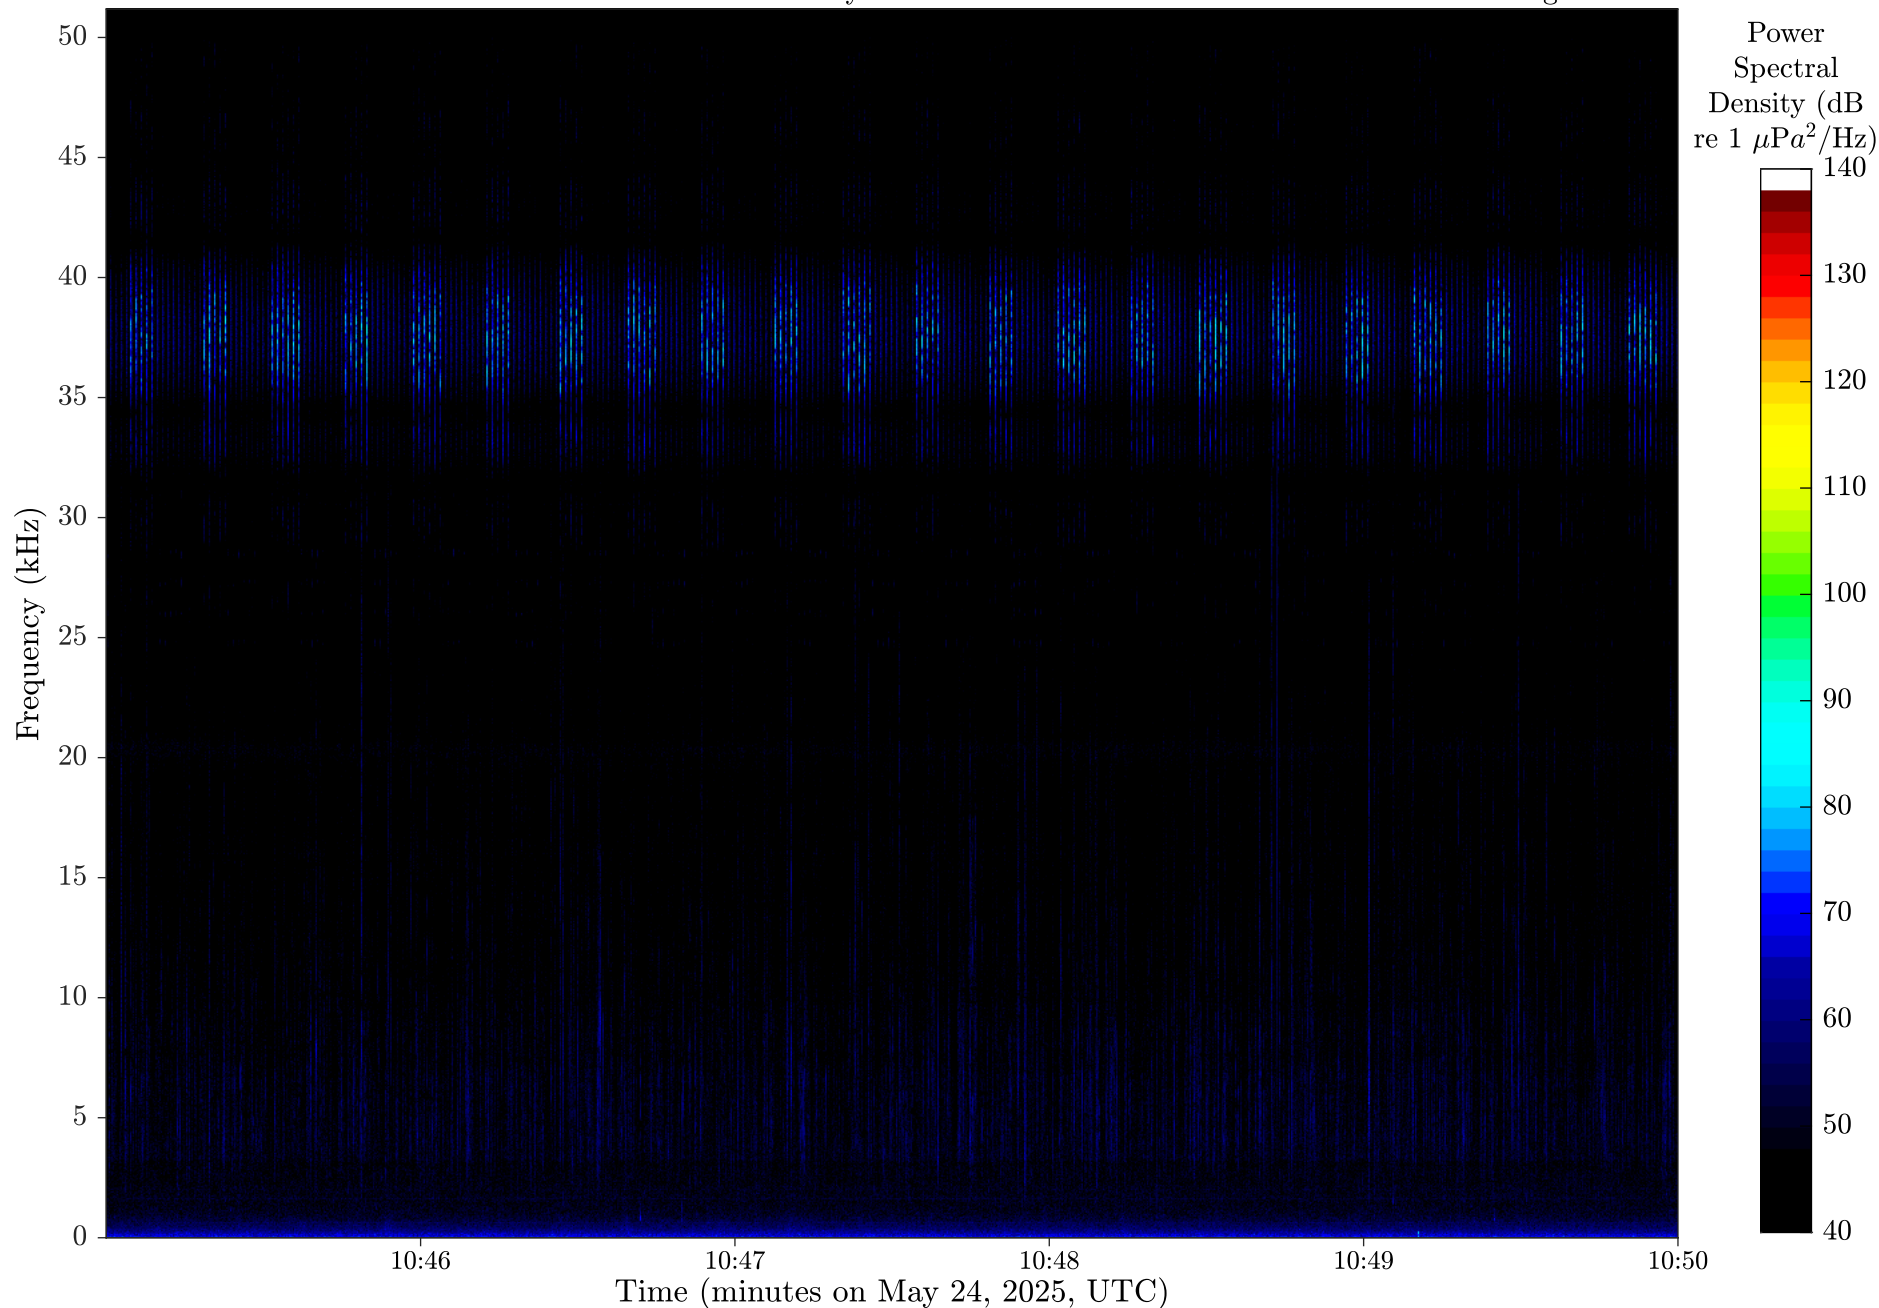


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:06 UTC

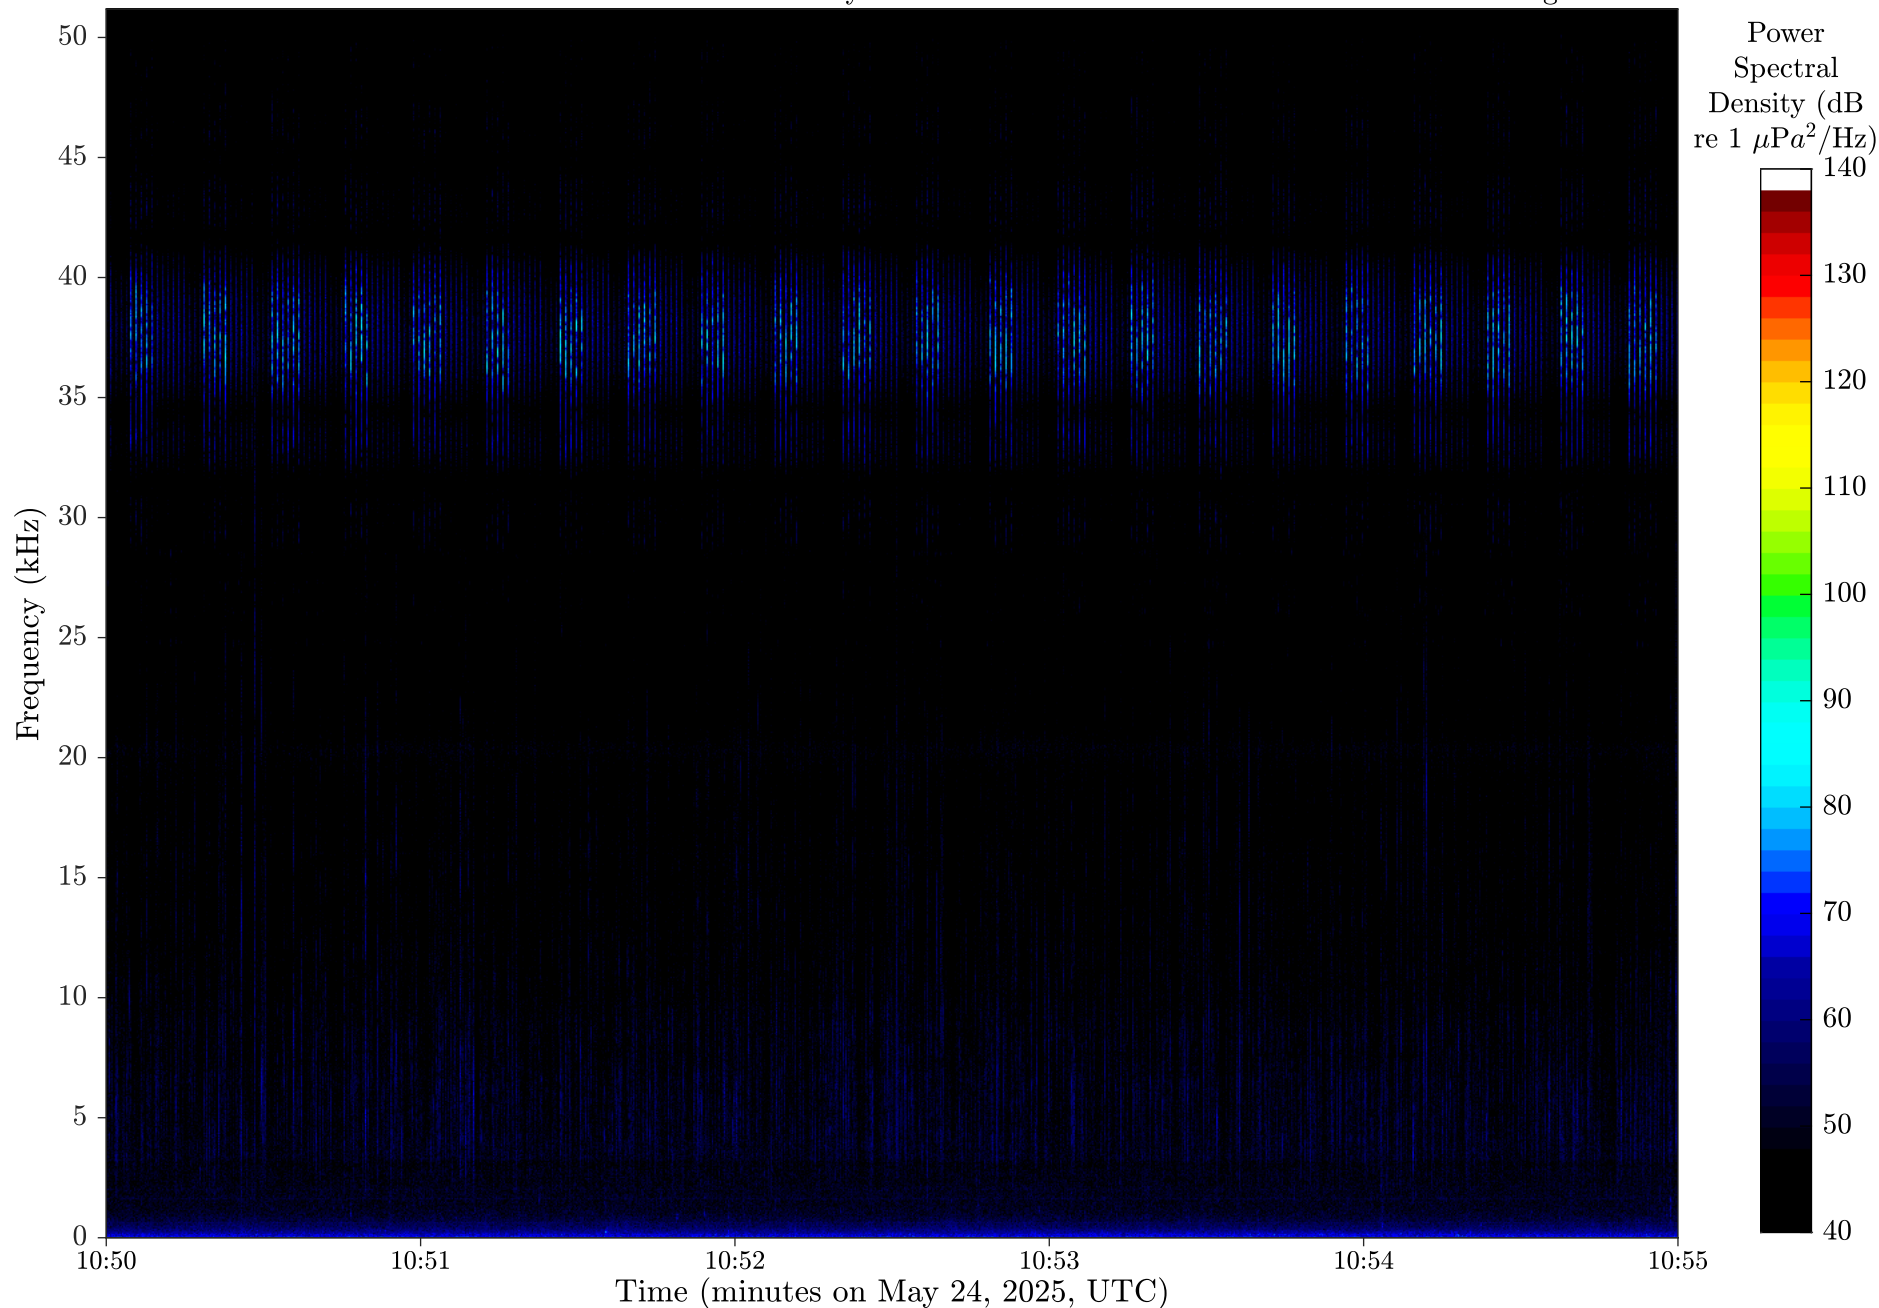


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:15 UTC

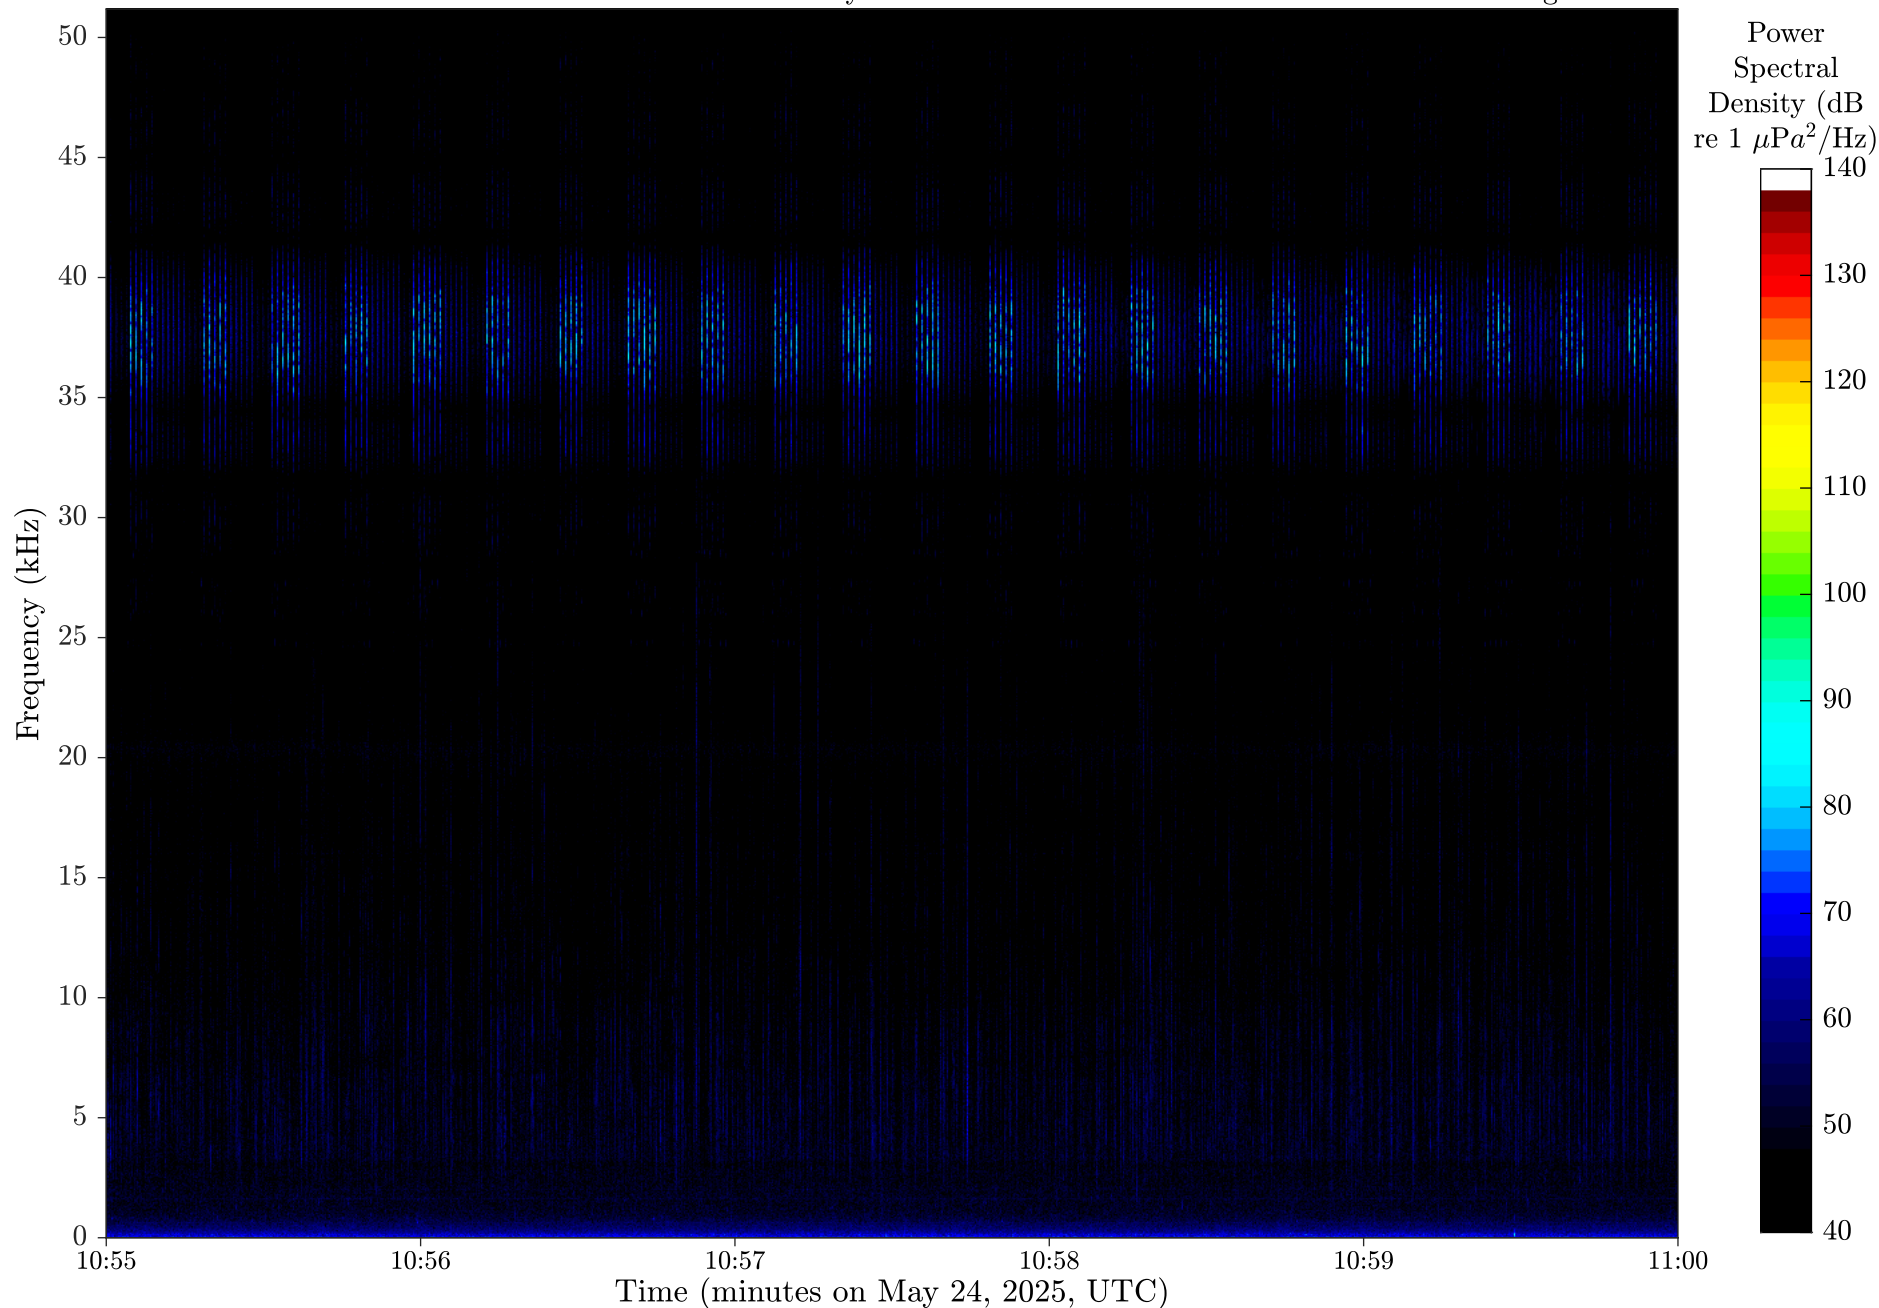

Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:25:23 UTC

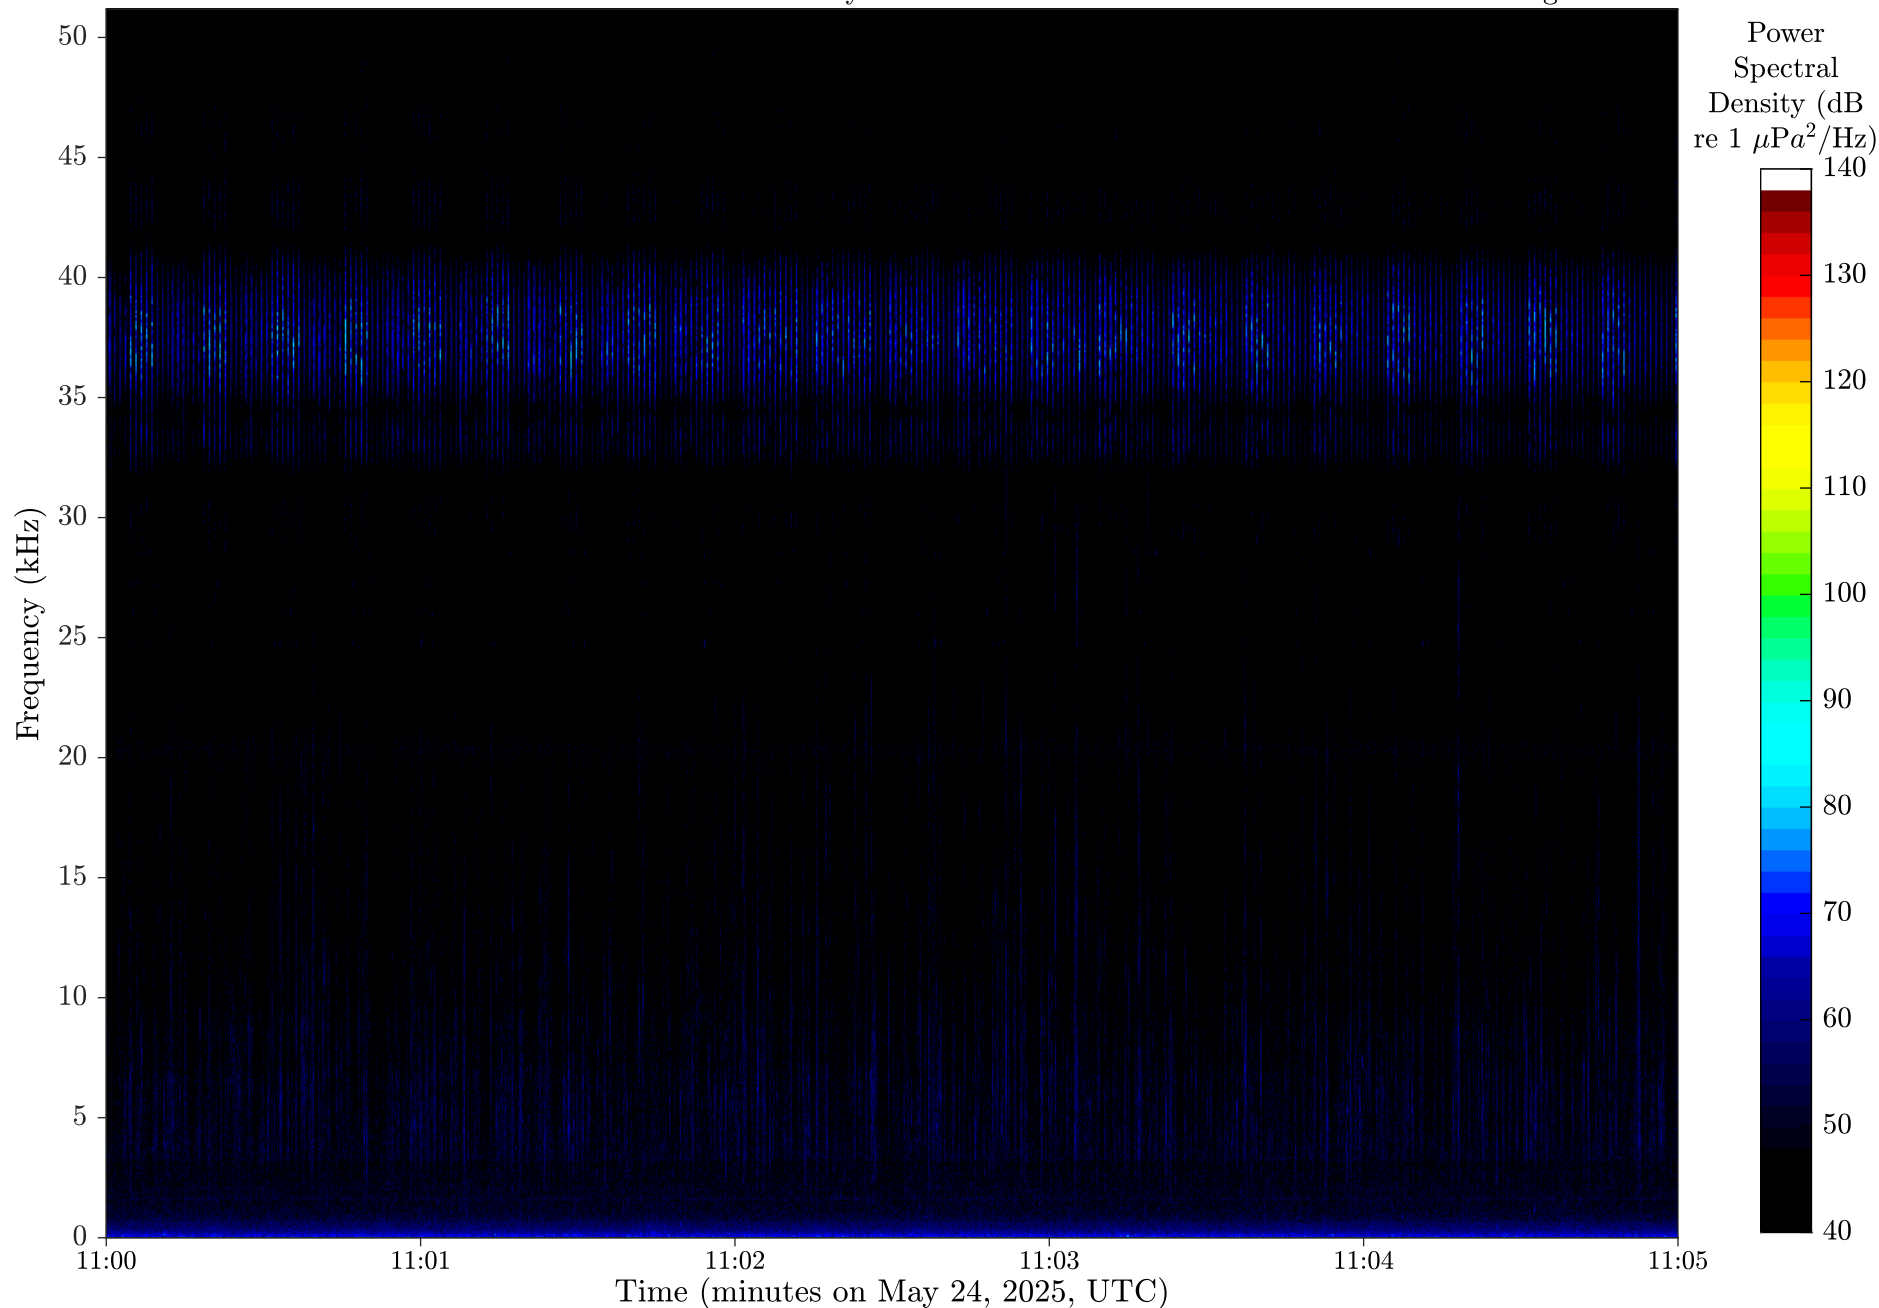


Ocean Sonics icListen HF Hydrophone 1266 (23235)
Folger Passage • Folger Deep • 48.8139° N • 125.2746° W • 95 m
Start time: 24-May-2025 11:05:00.000 UTC • Data Diversion Mode: Original Data




Comments: 23.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

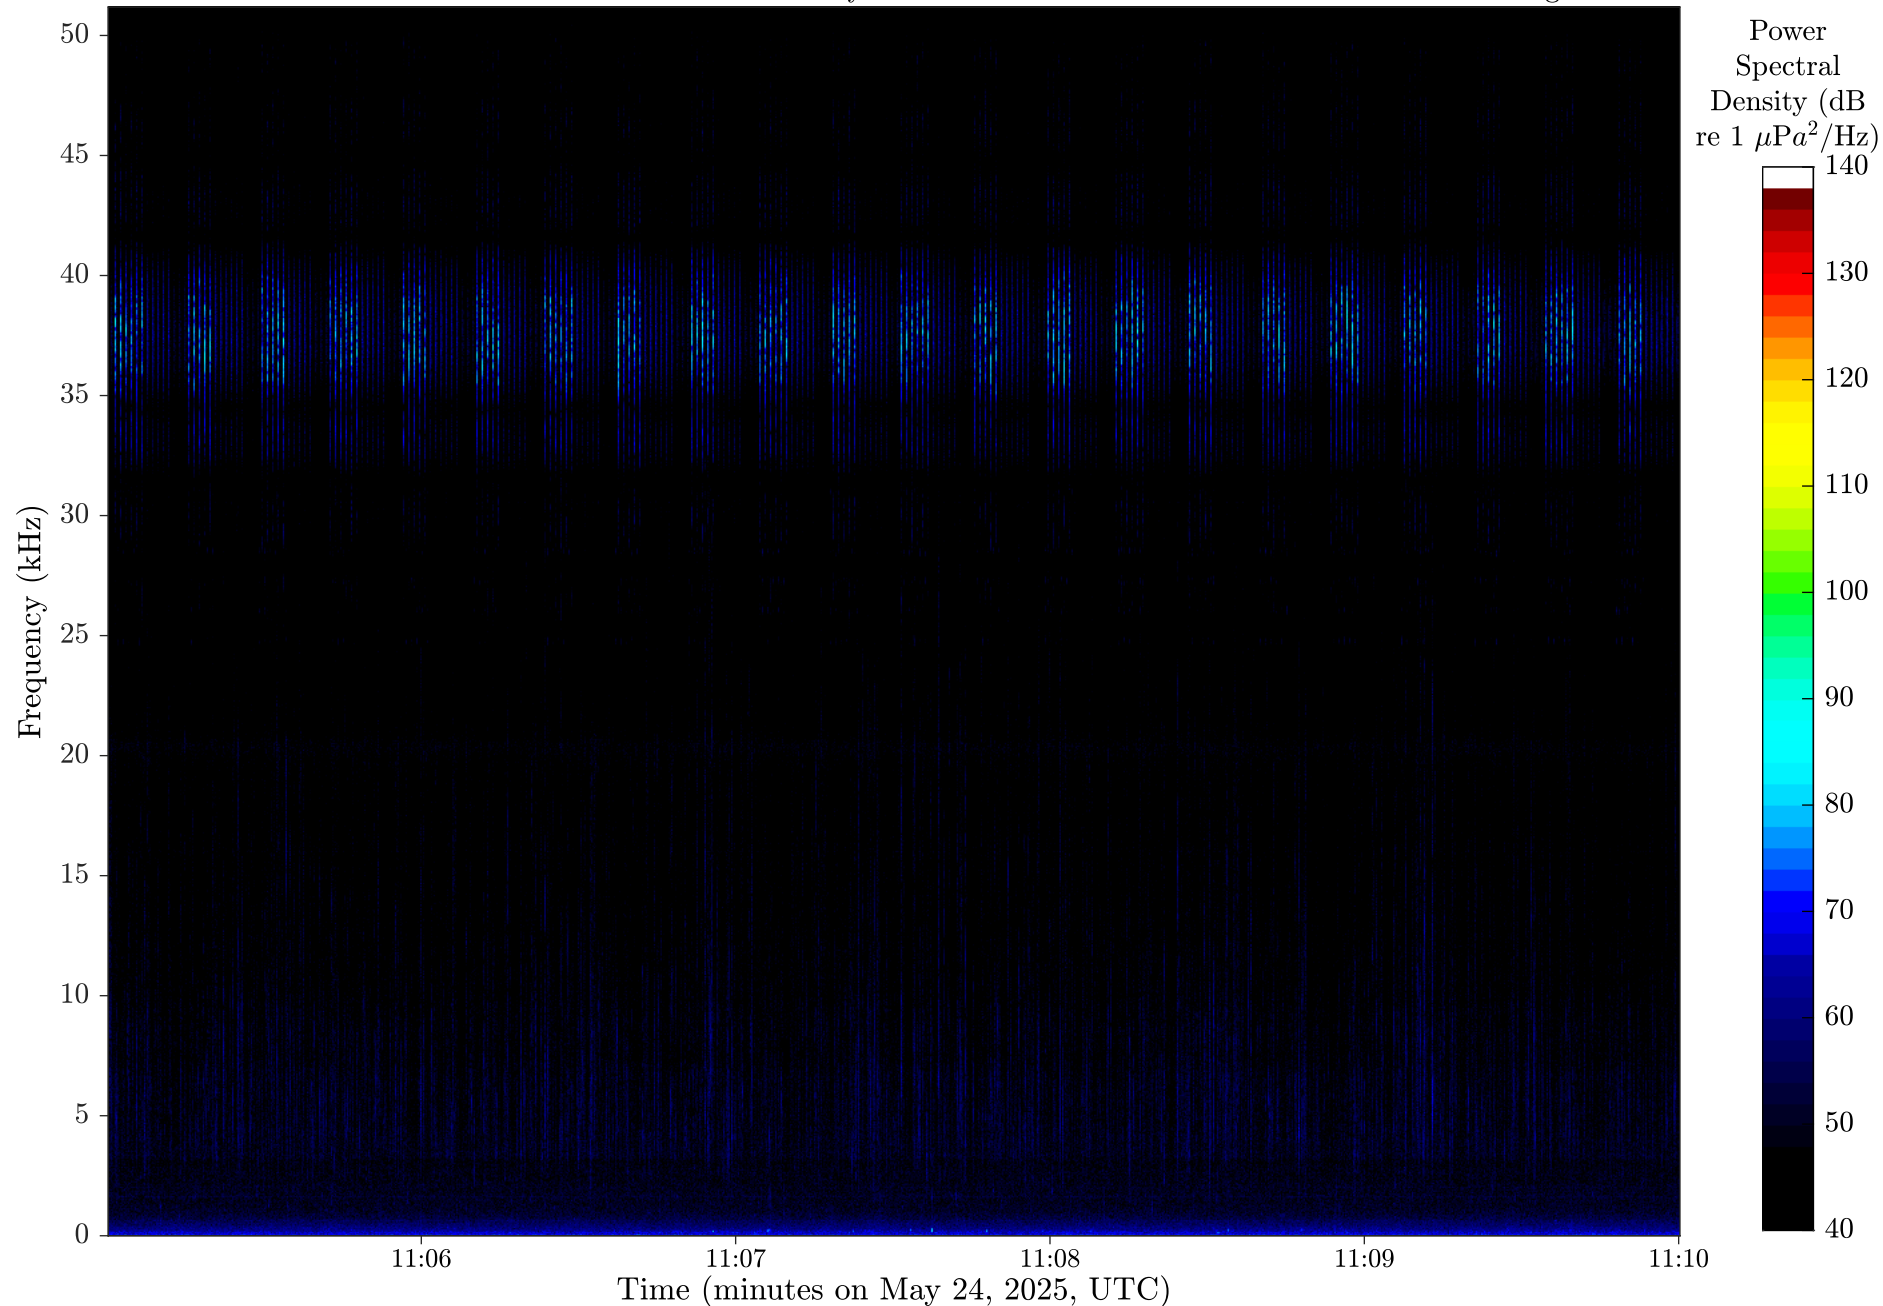

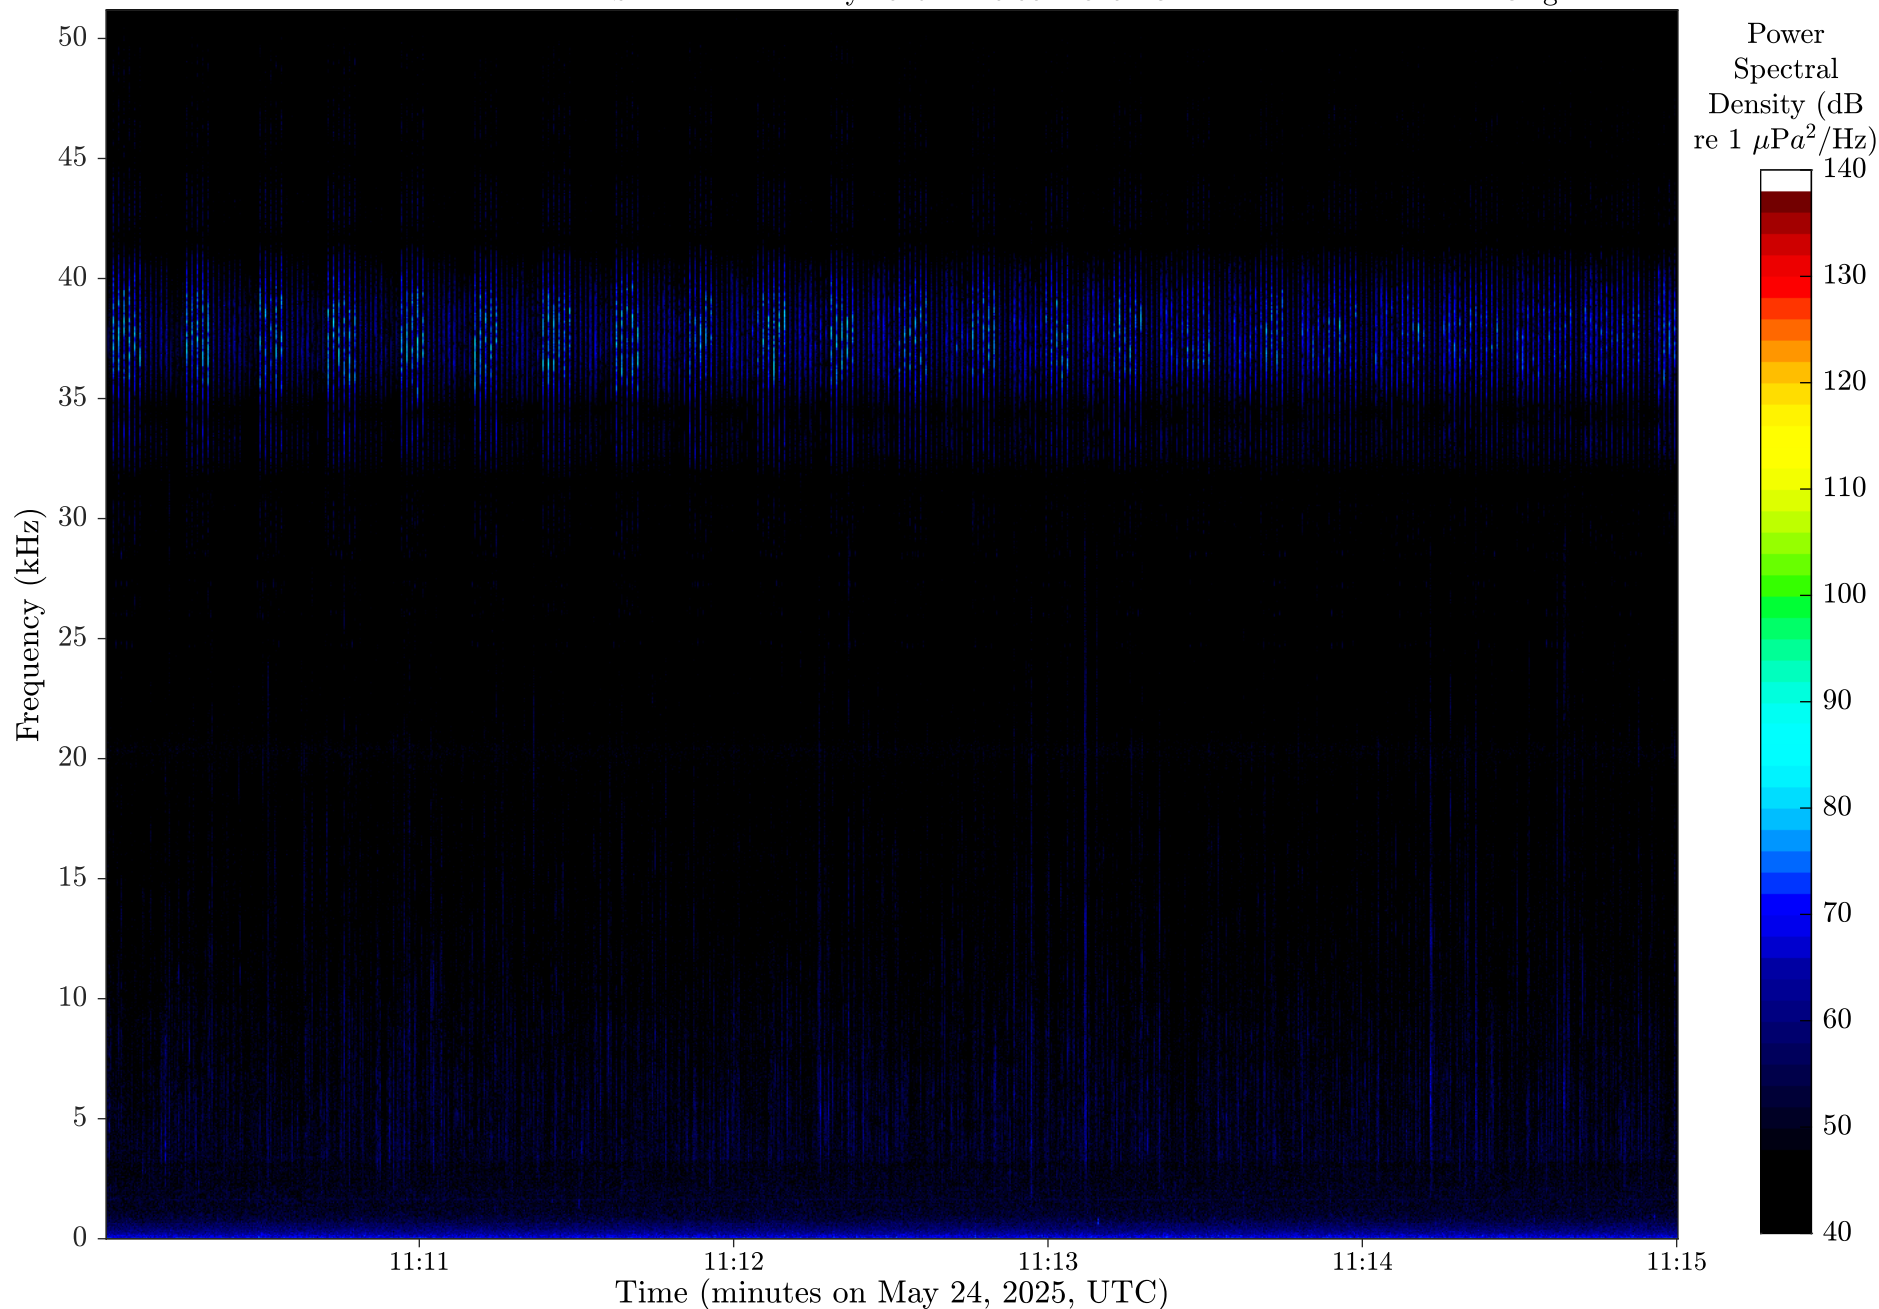


Comments: 32.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:50 UTC

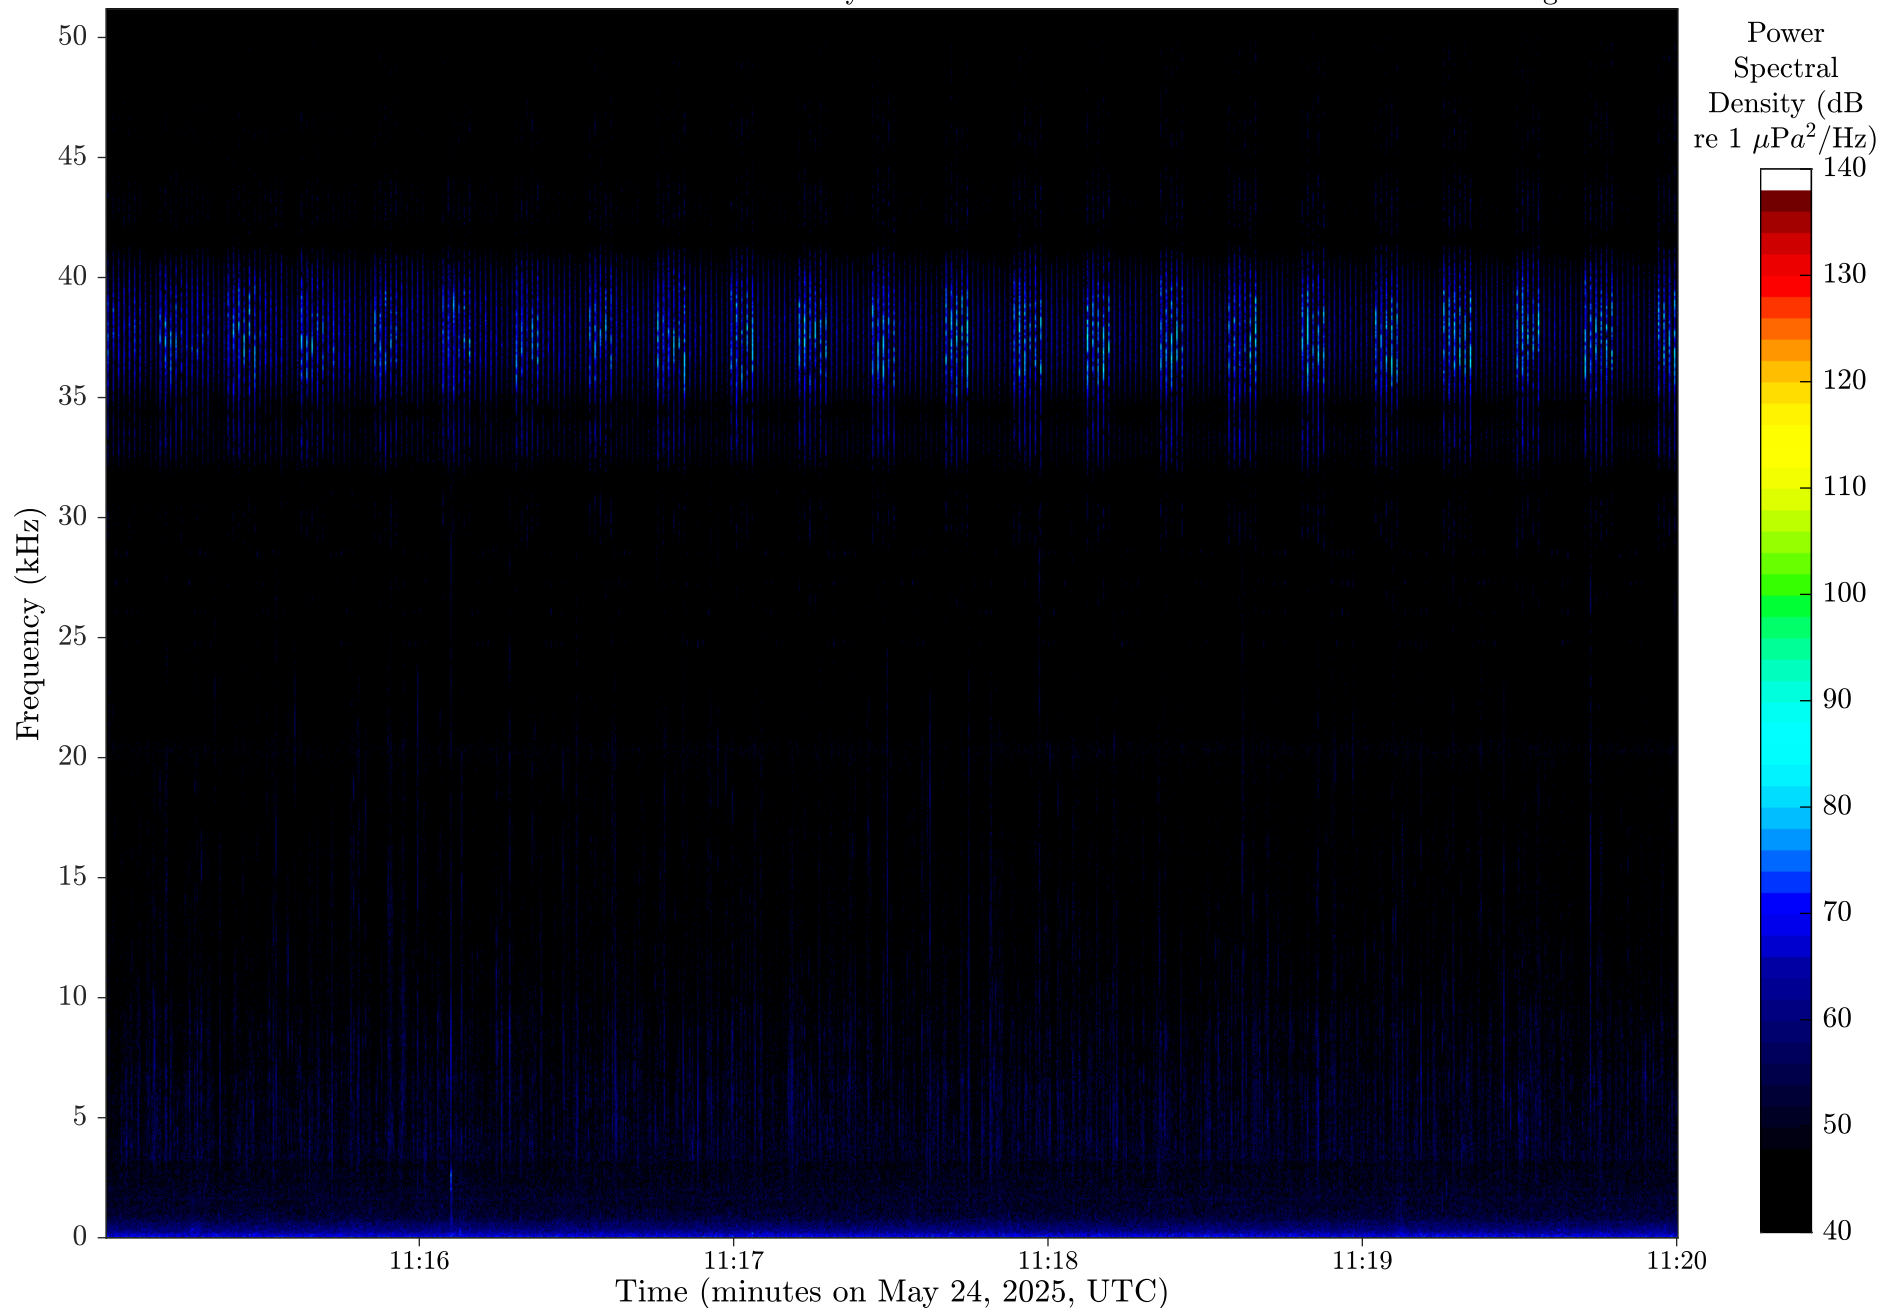


Comments: 31.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:59 UTC

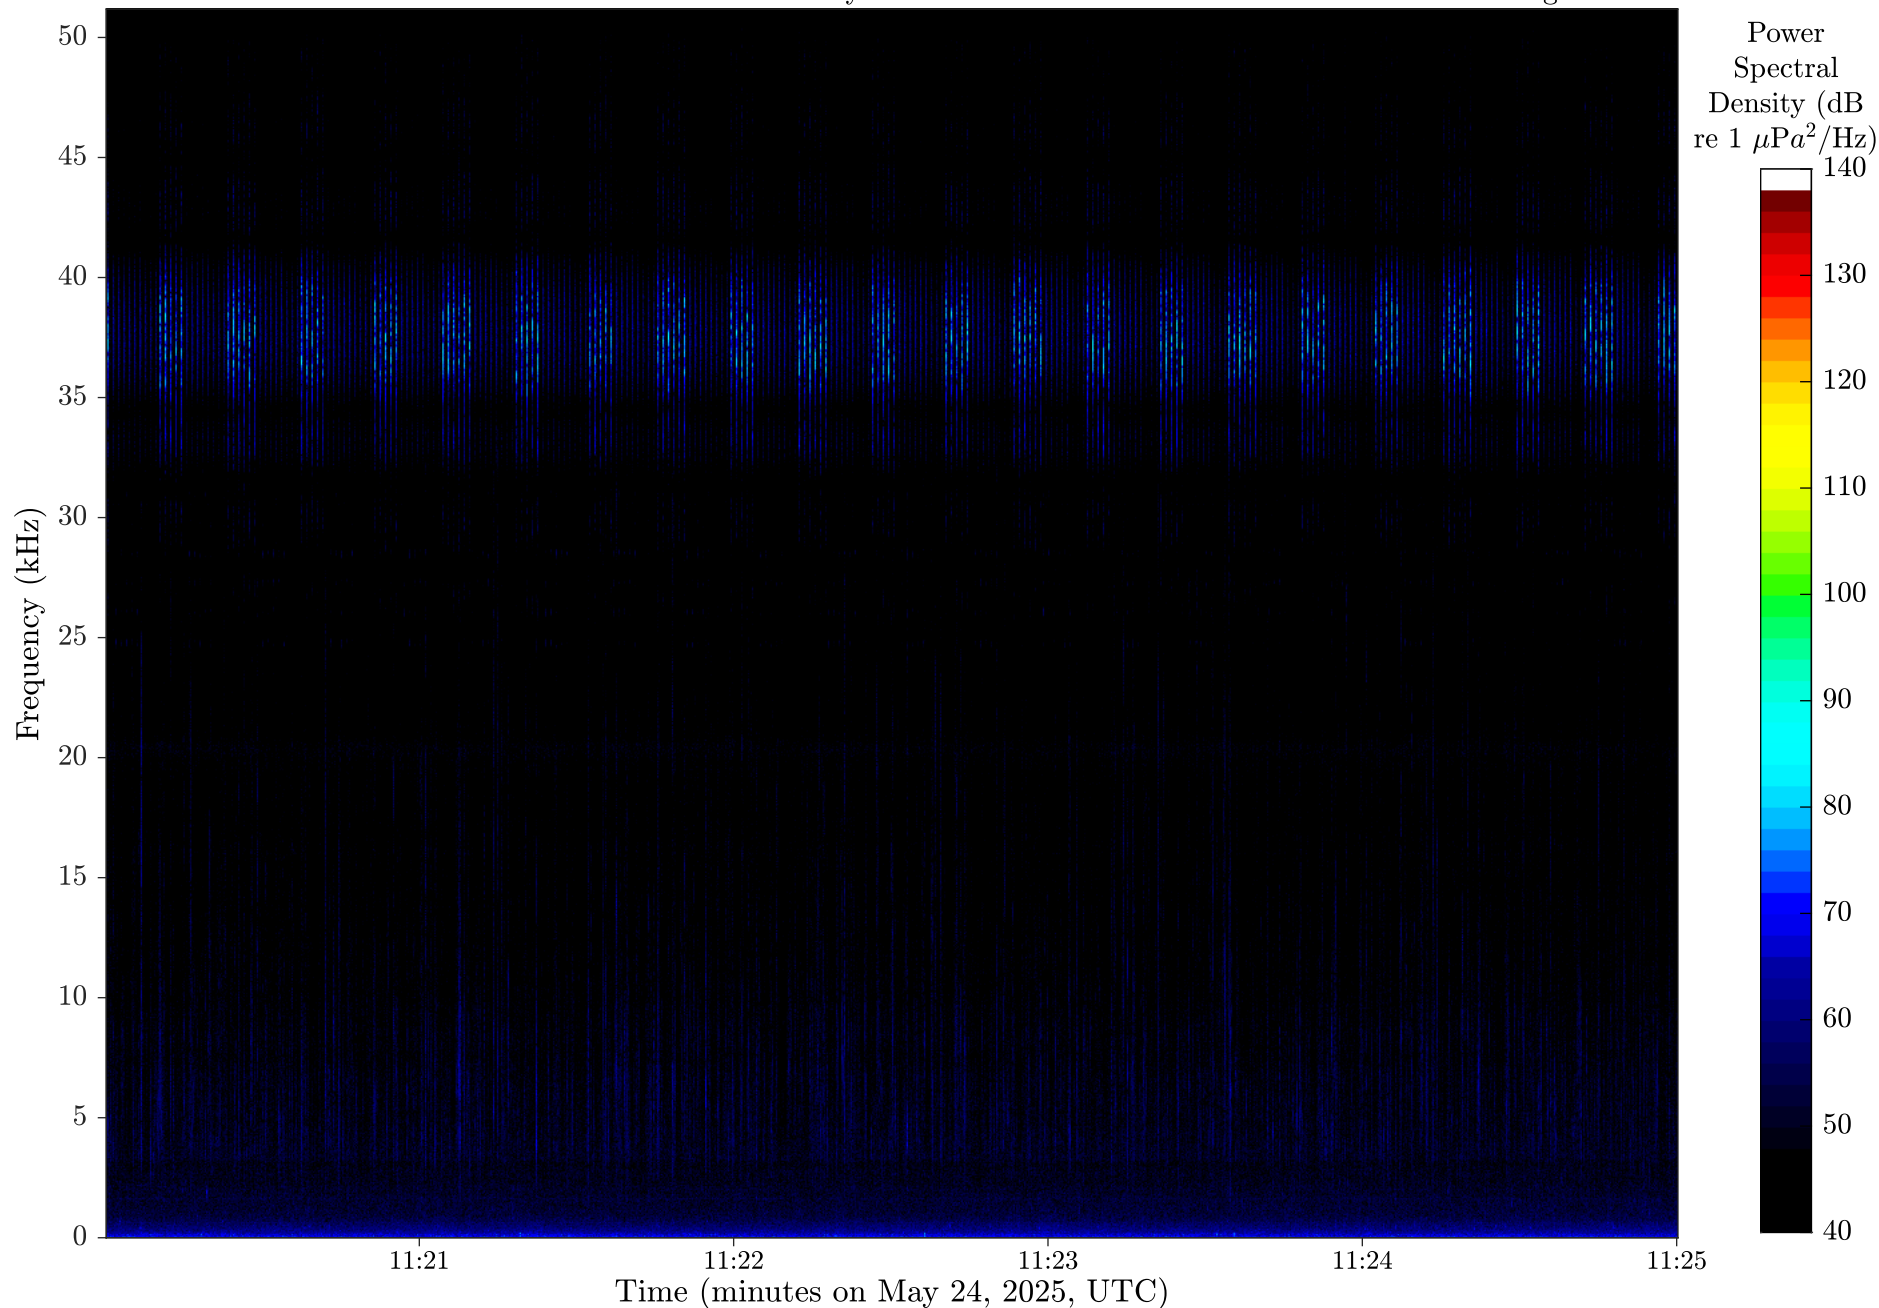


Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:26:07 UTC

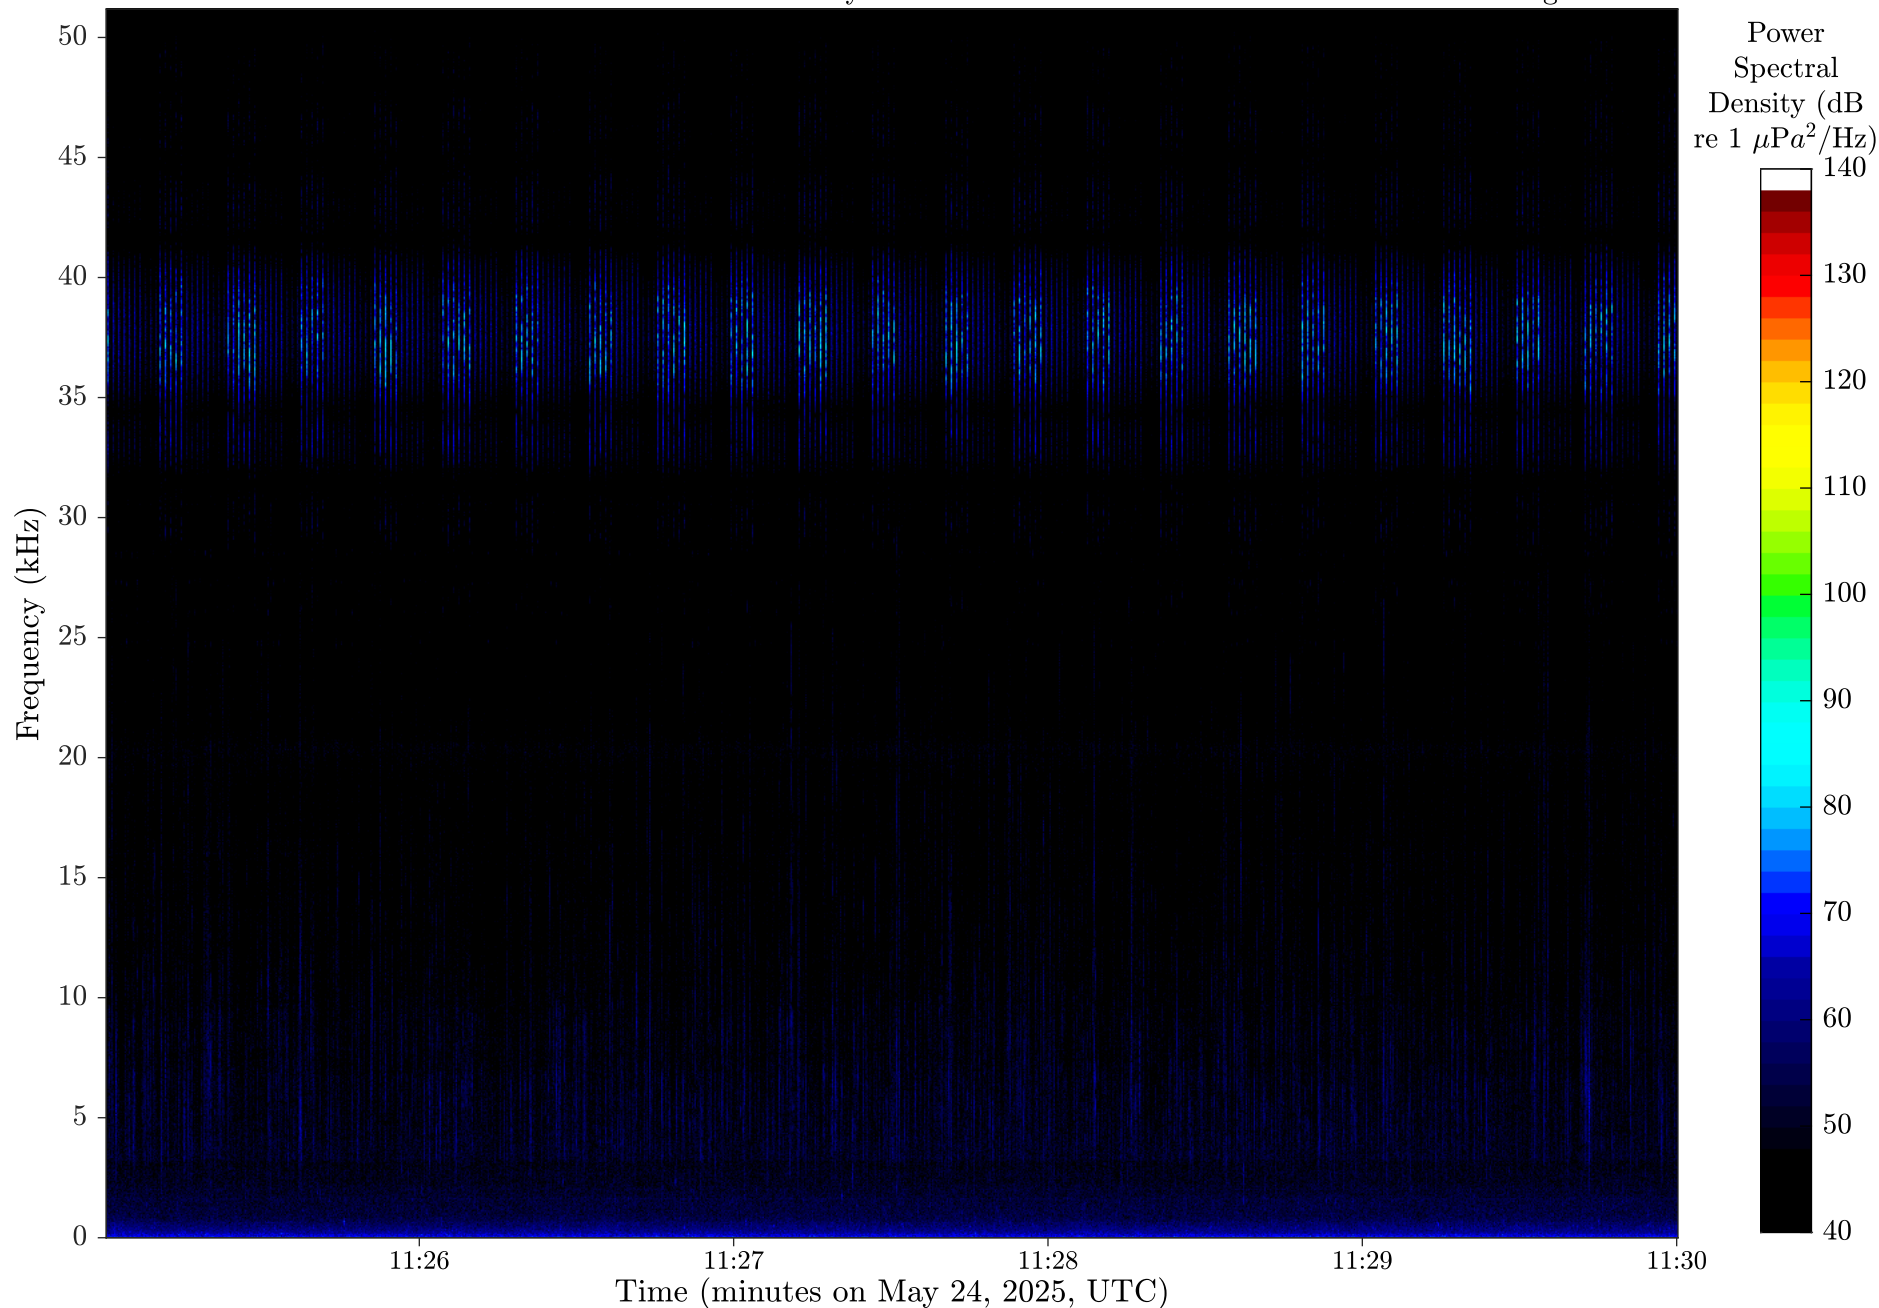


Comments: 32.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:26:15 UTC

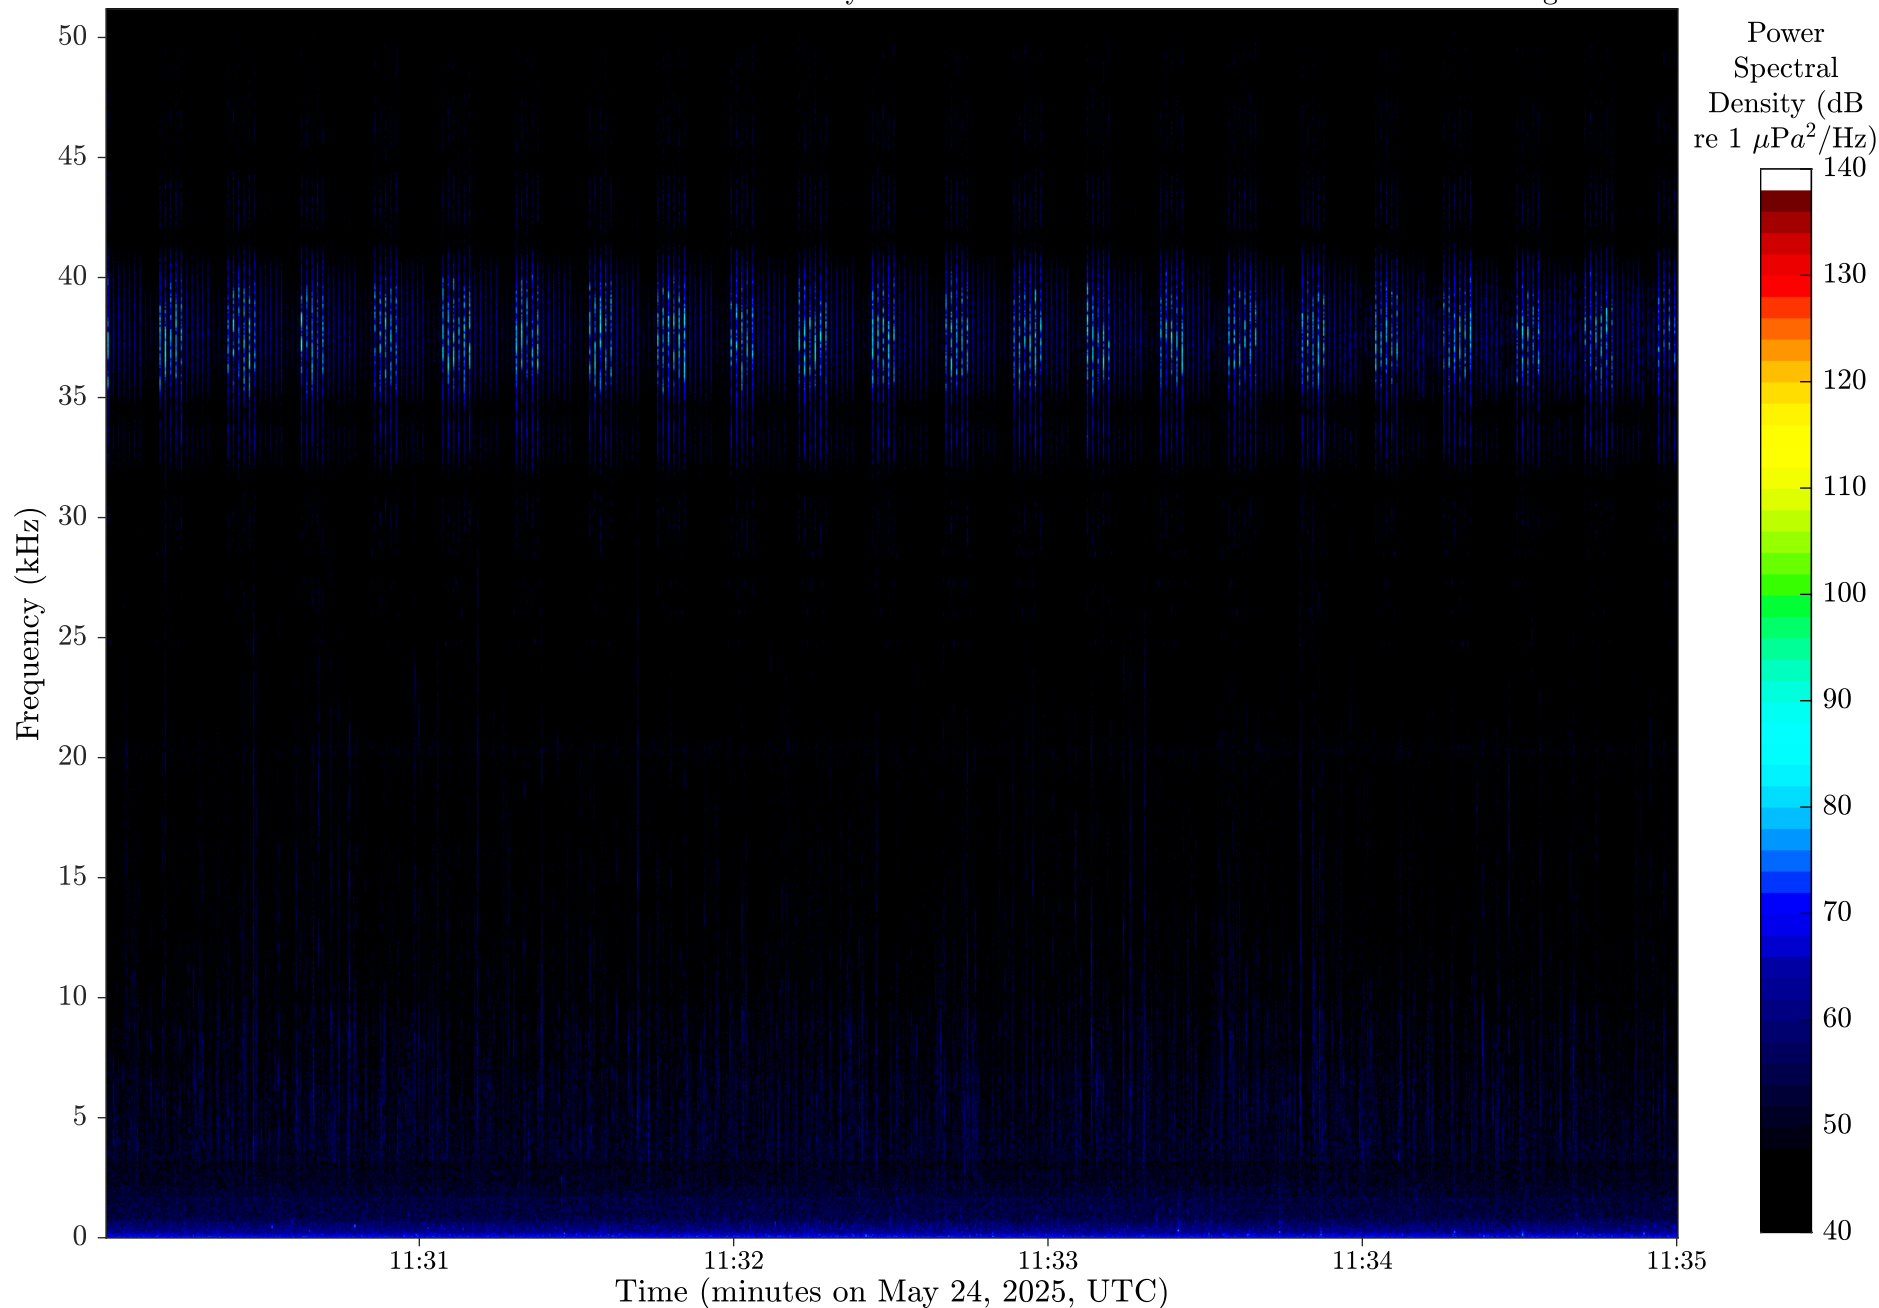


Comments: 32.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:26:23 UTC

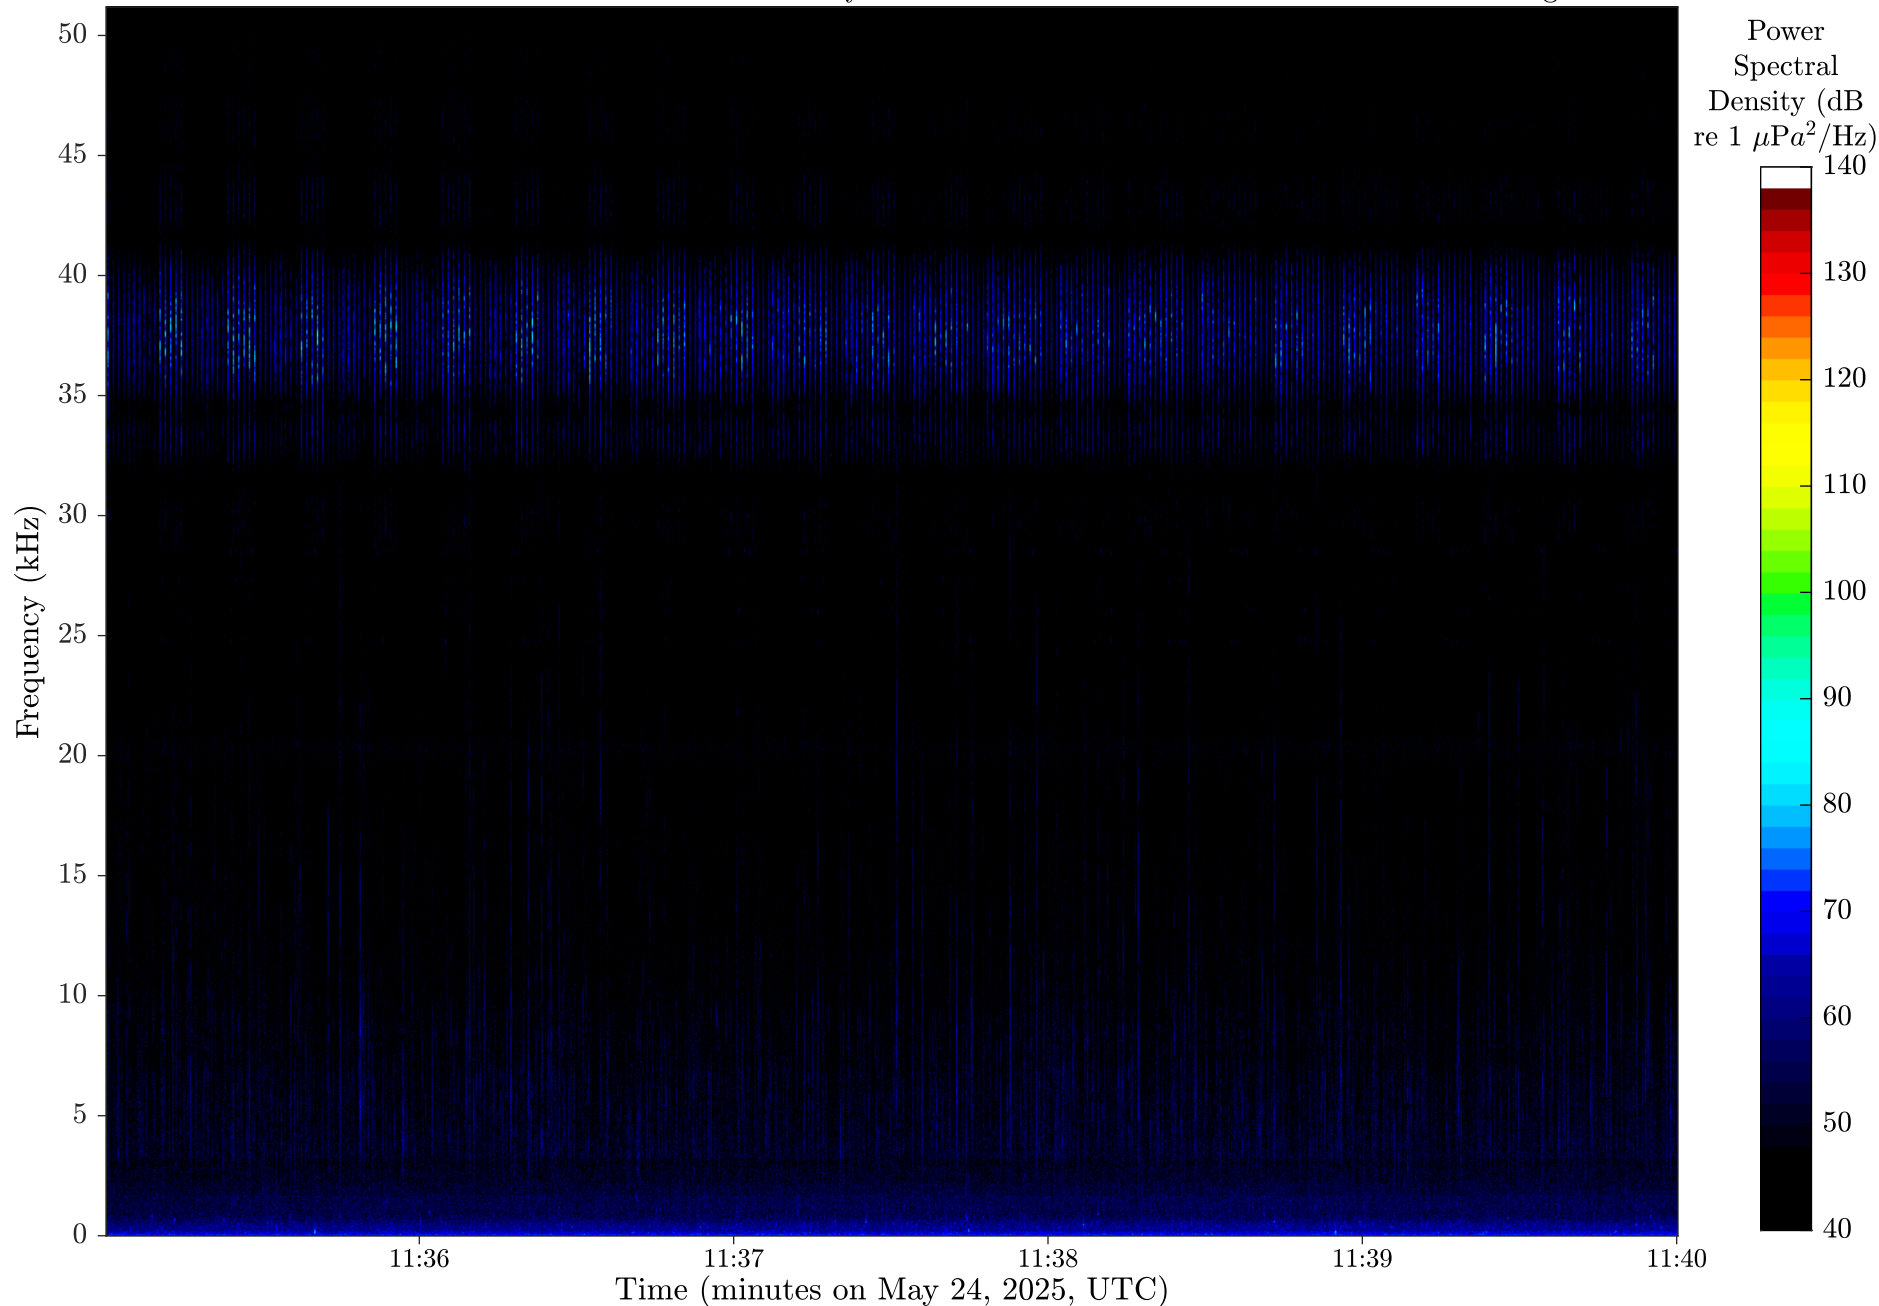


Comments: 30.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:26:31 UTC

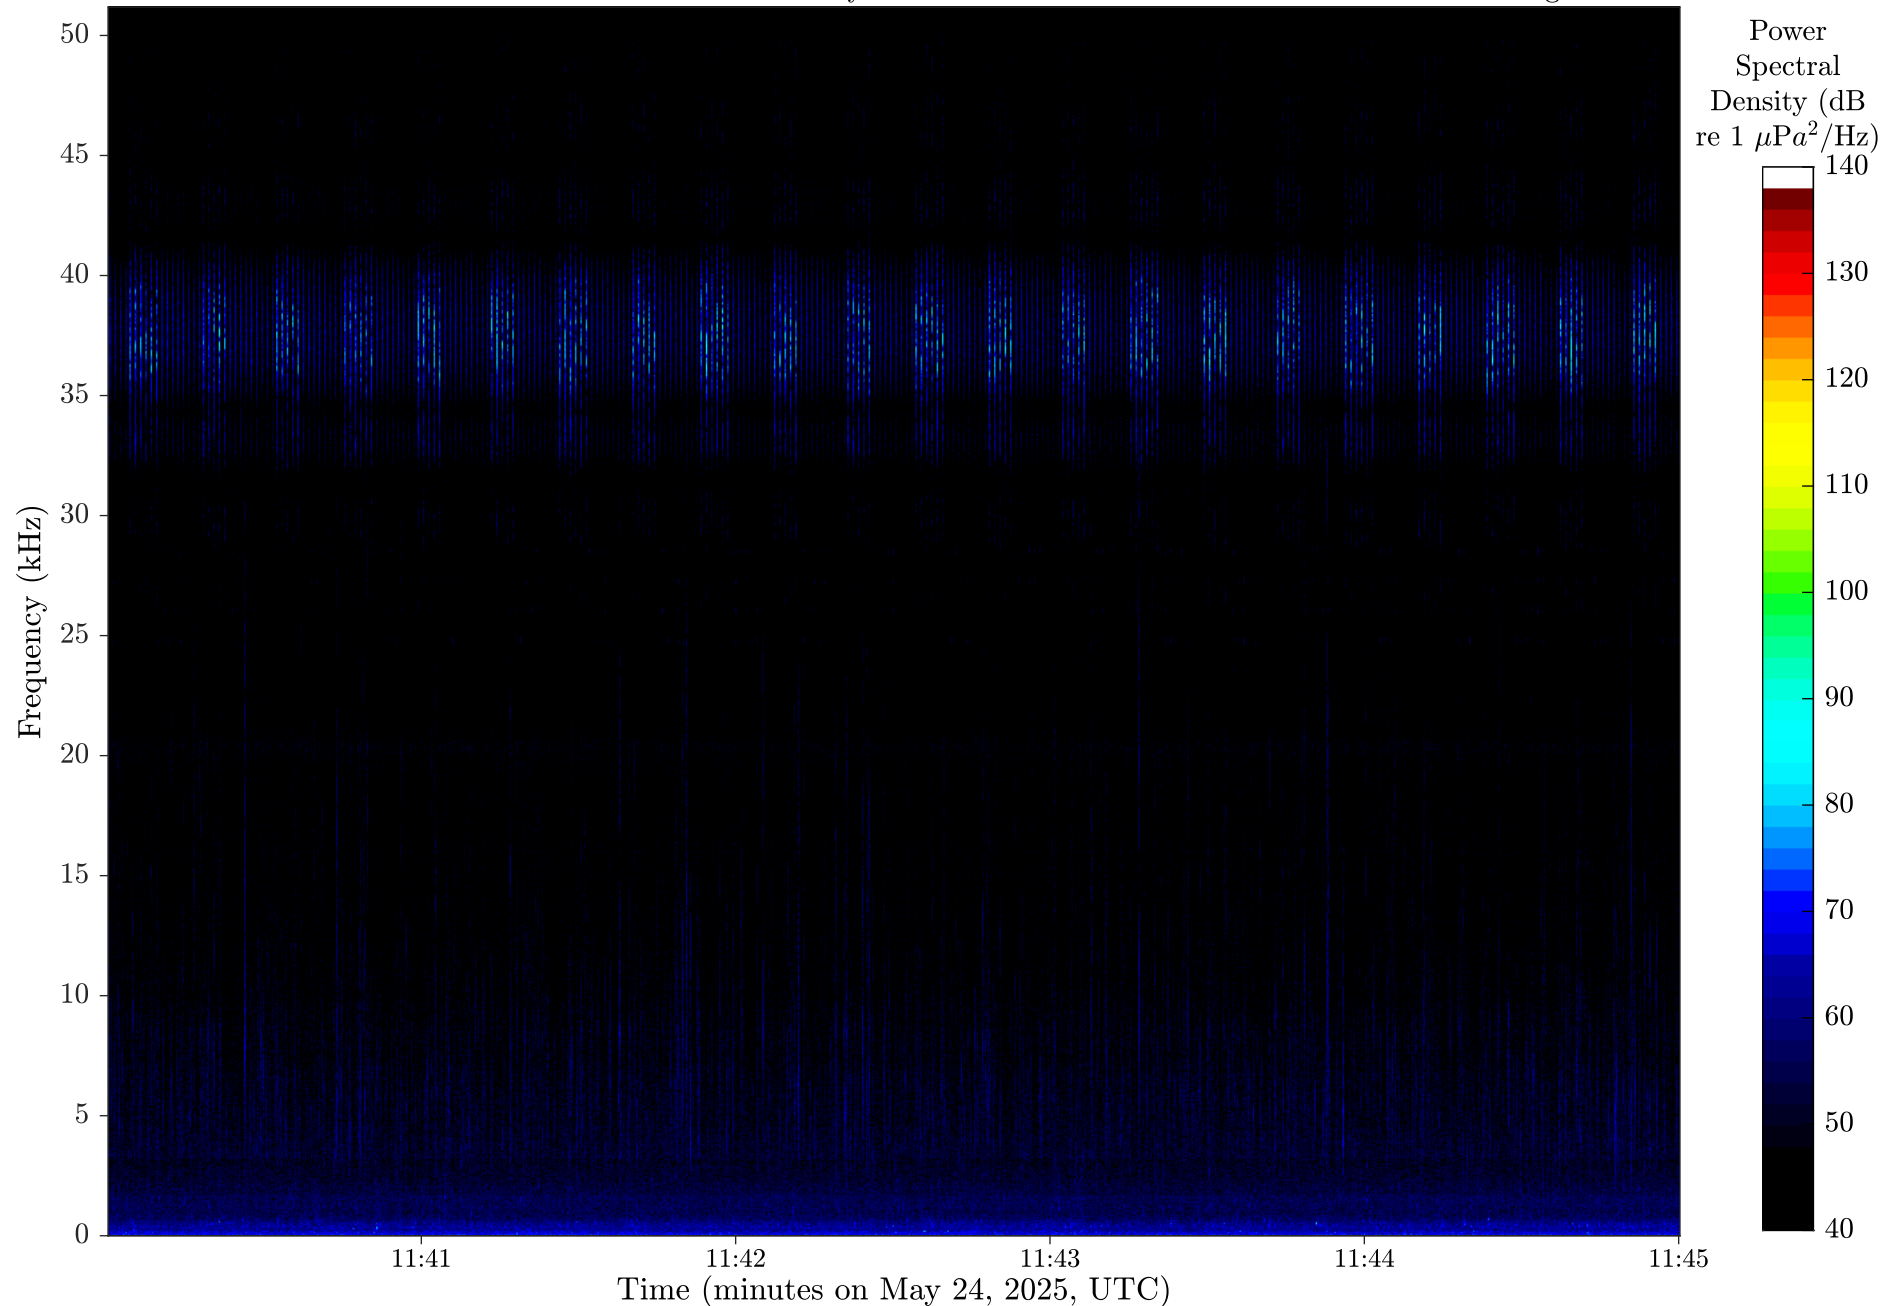

Comments: 30.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:26:38 UTC

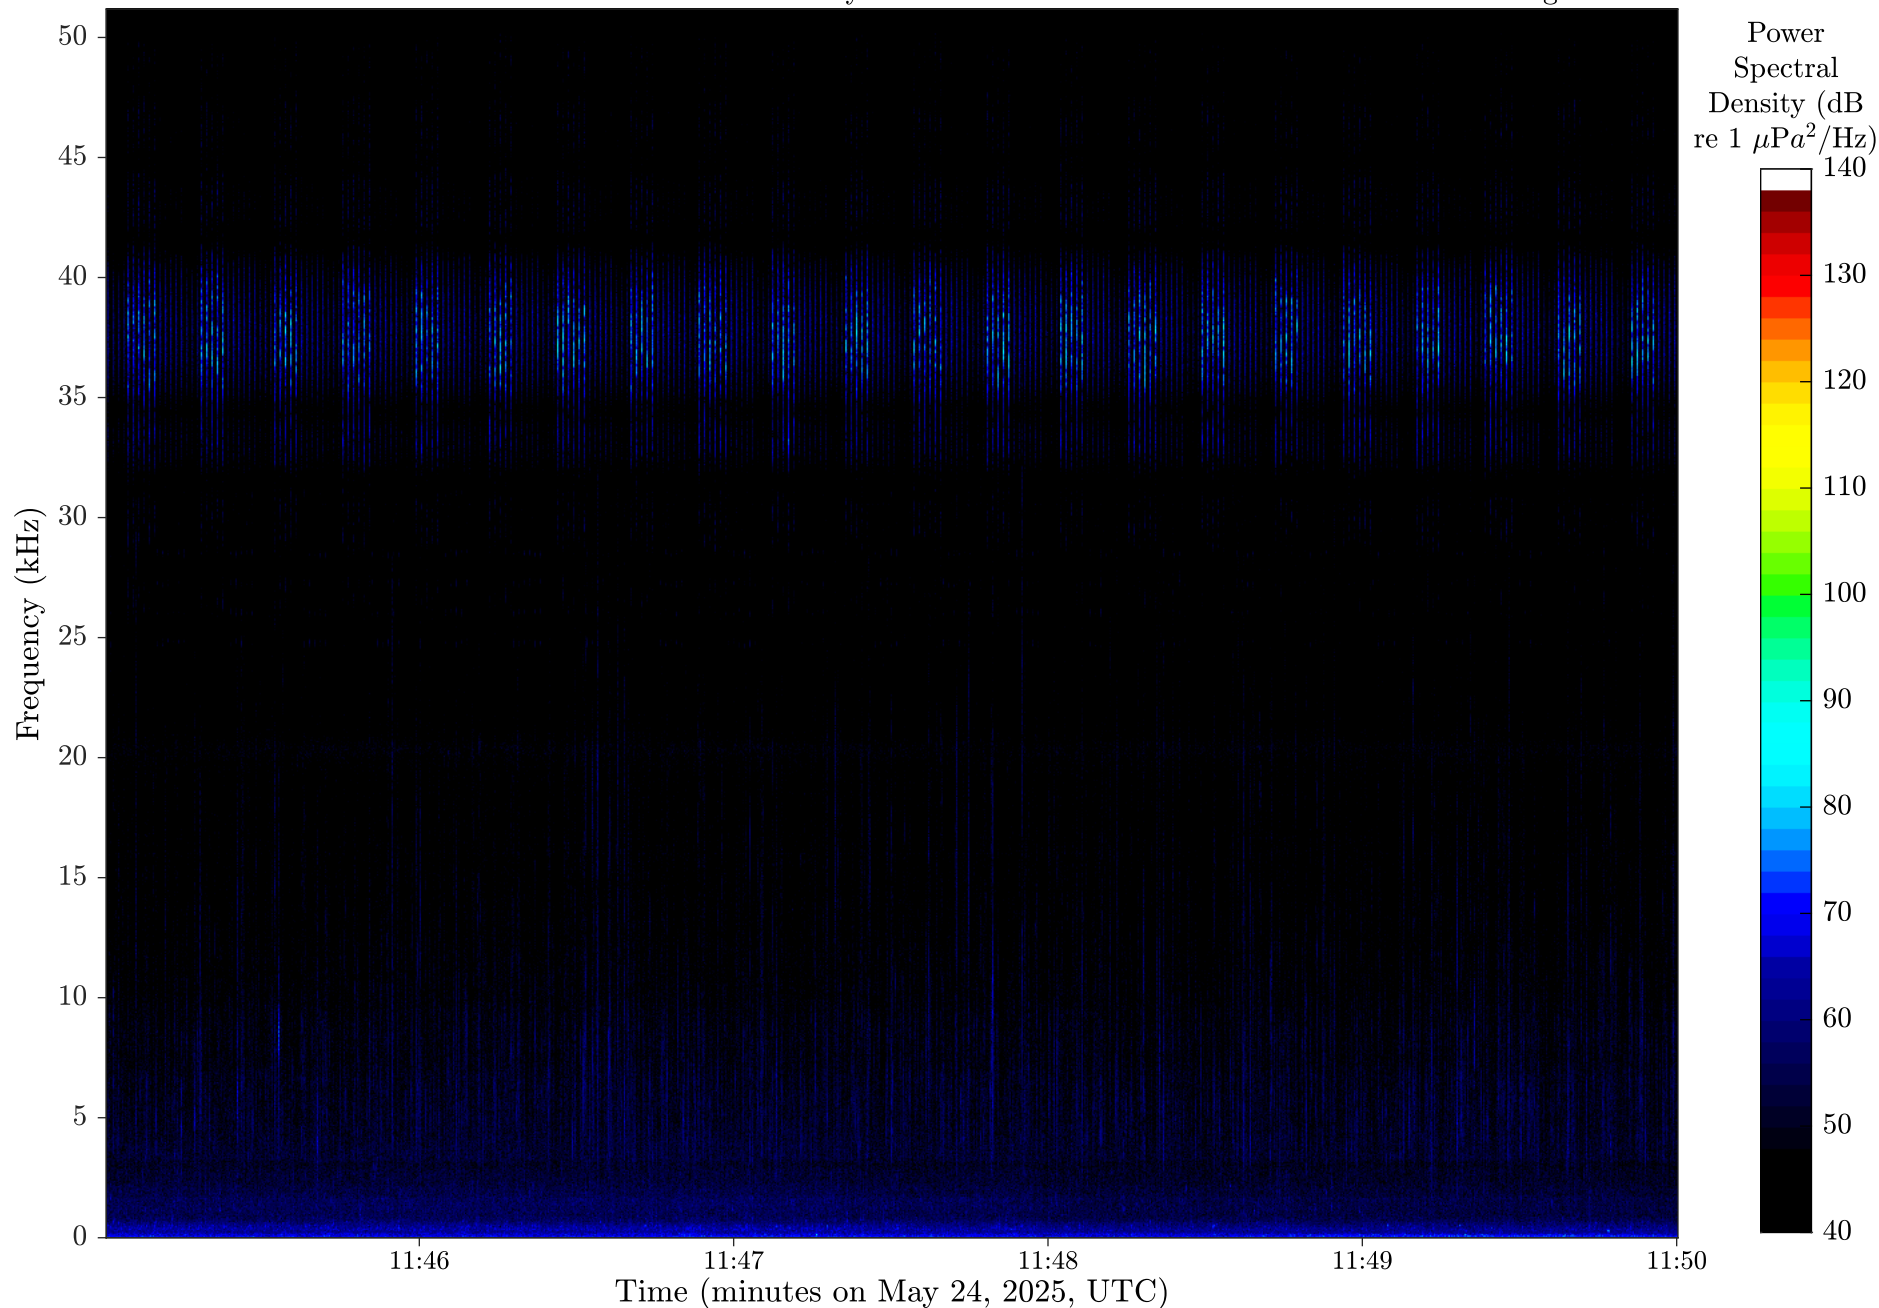


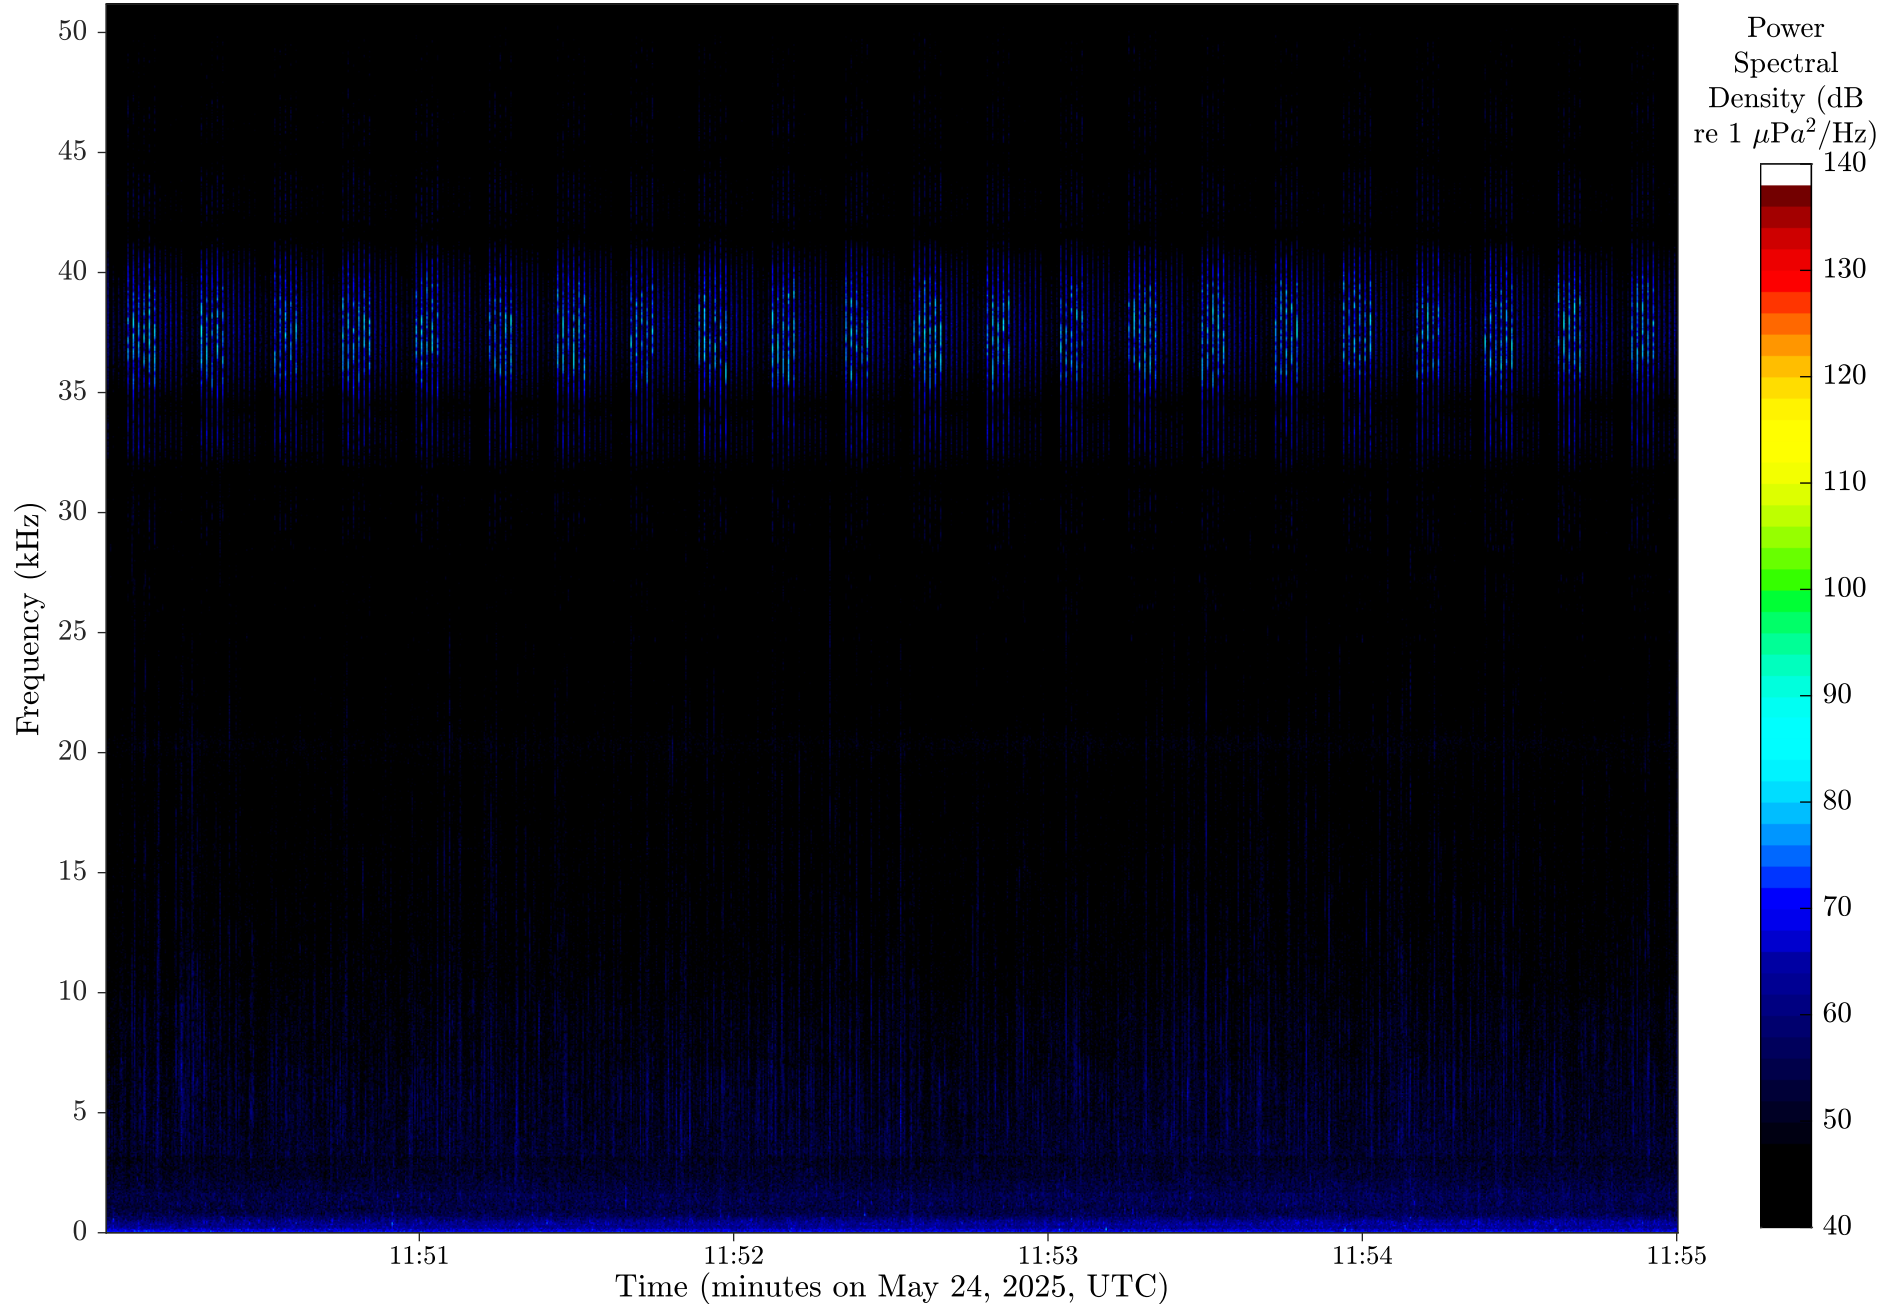


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:26:52 UTC

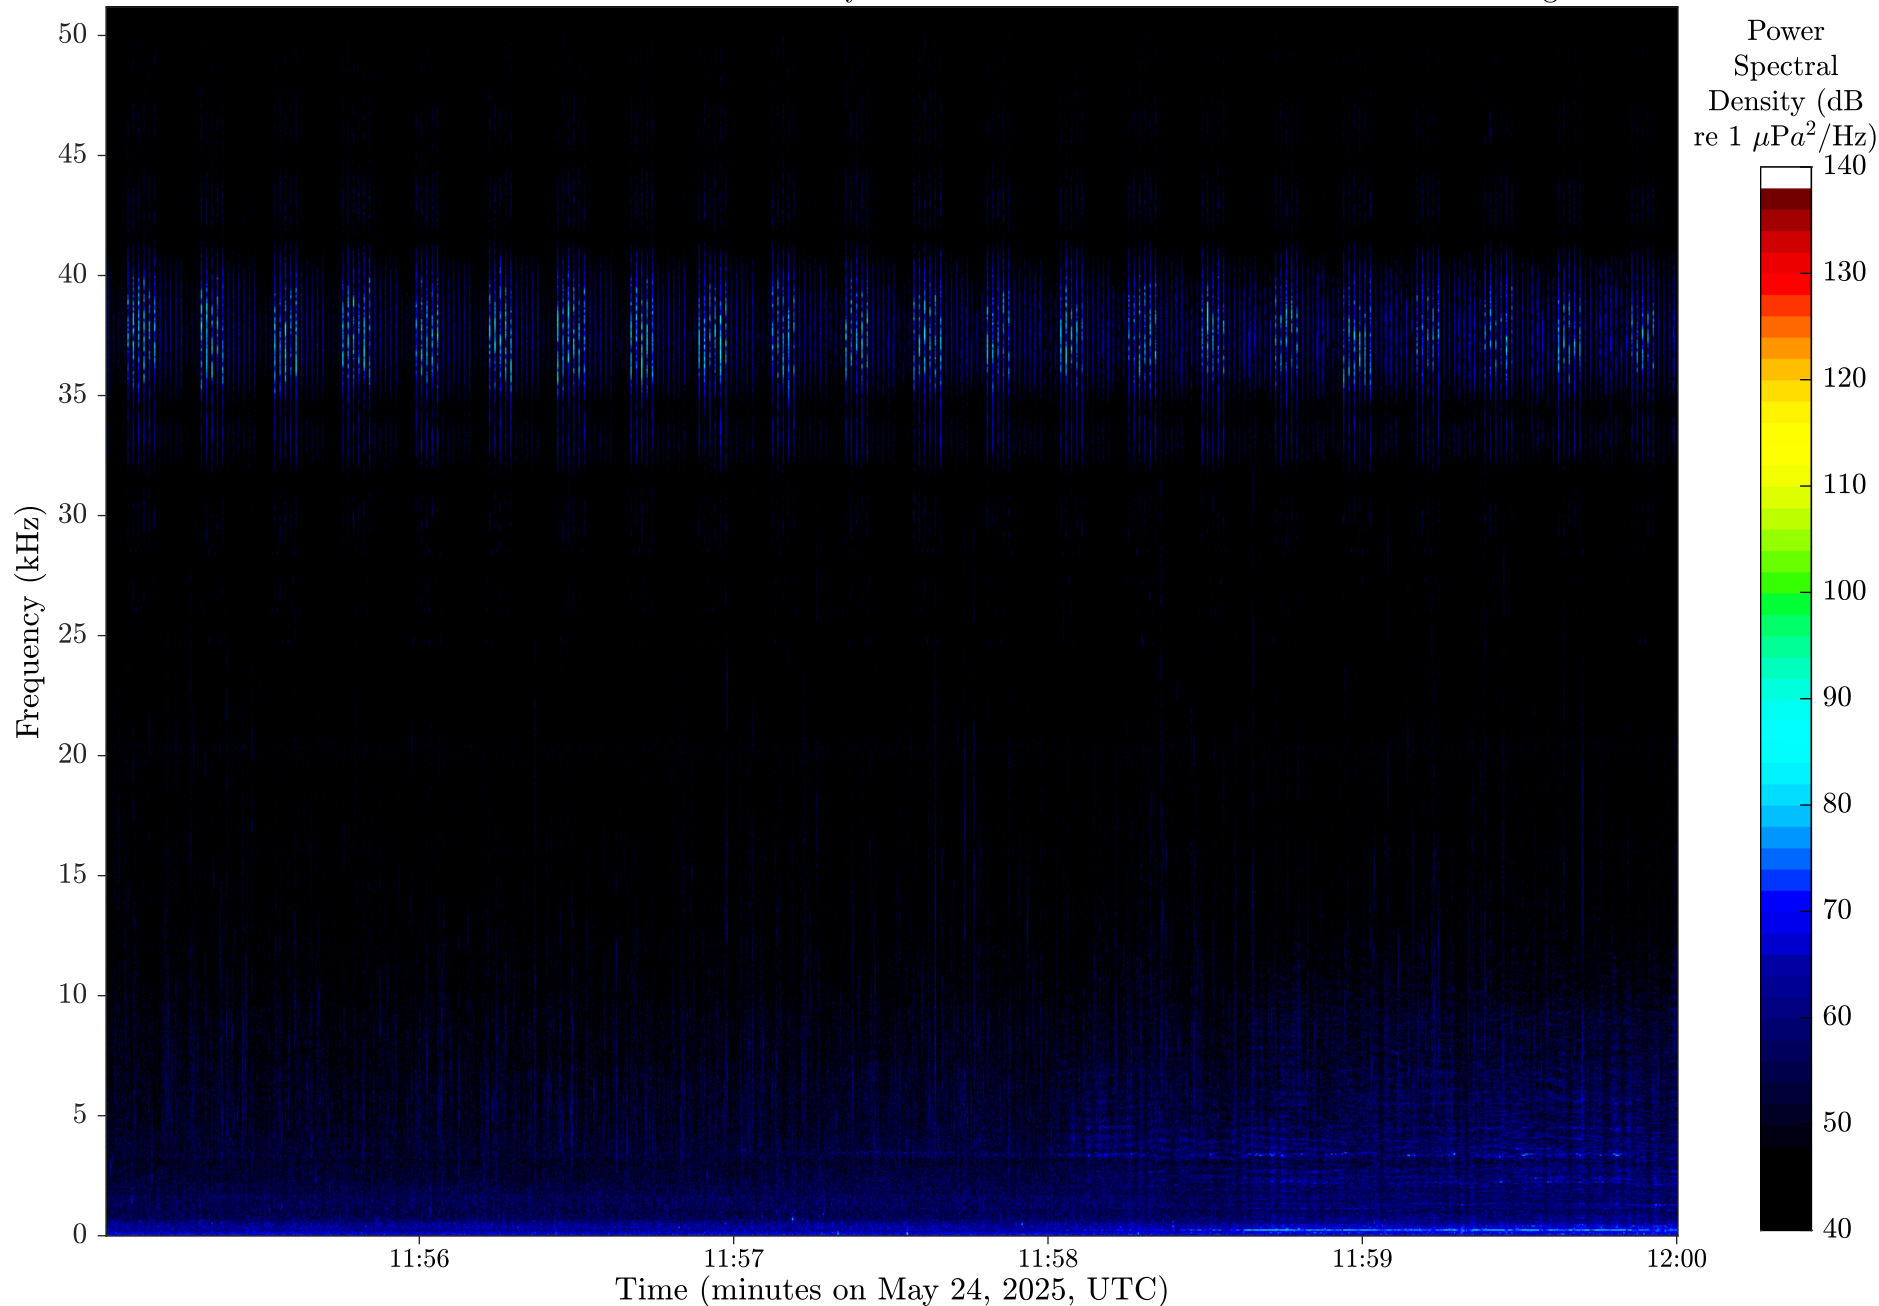


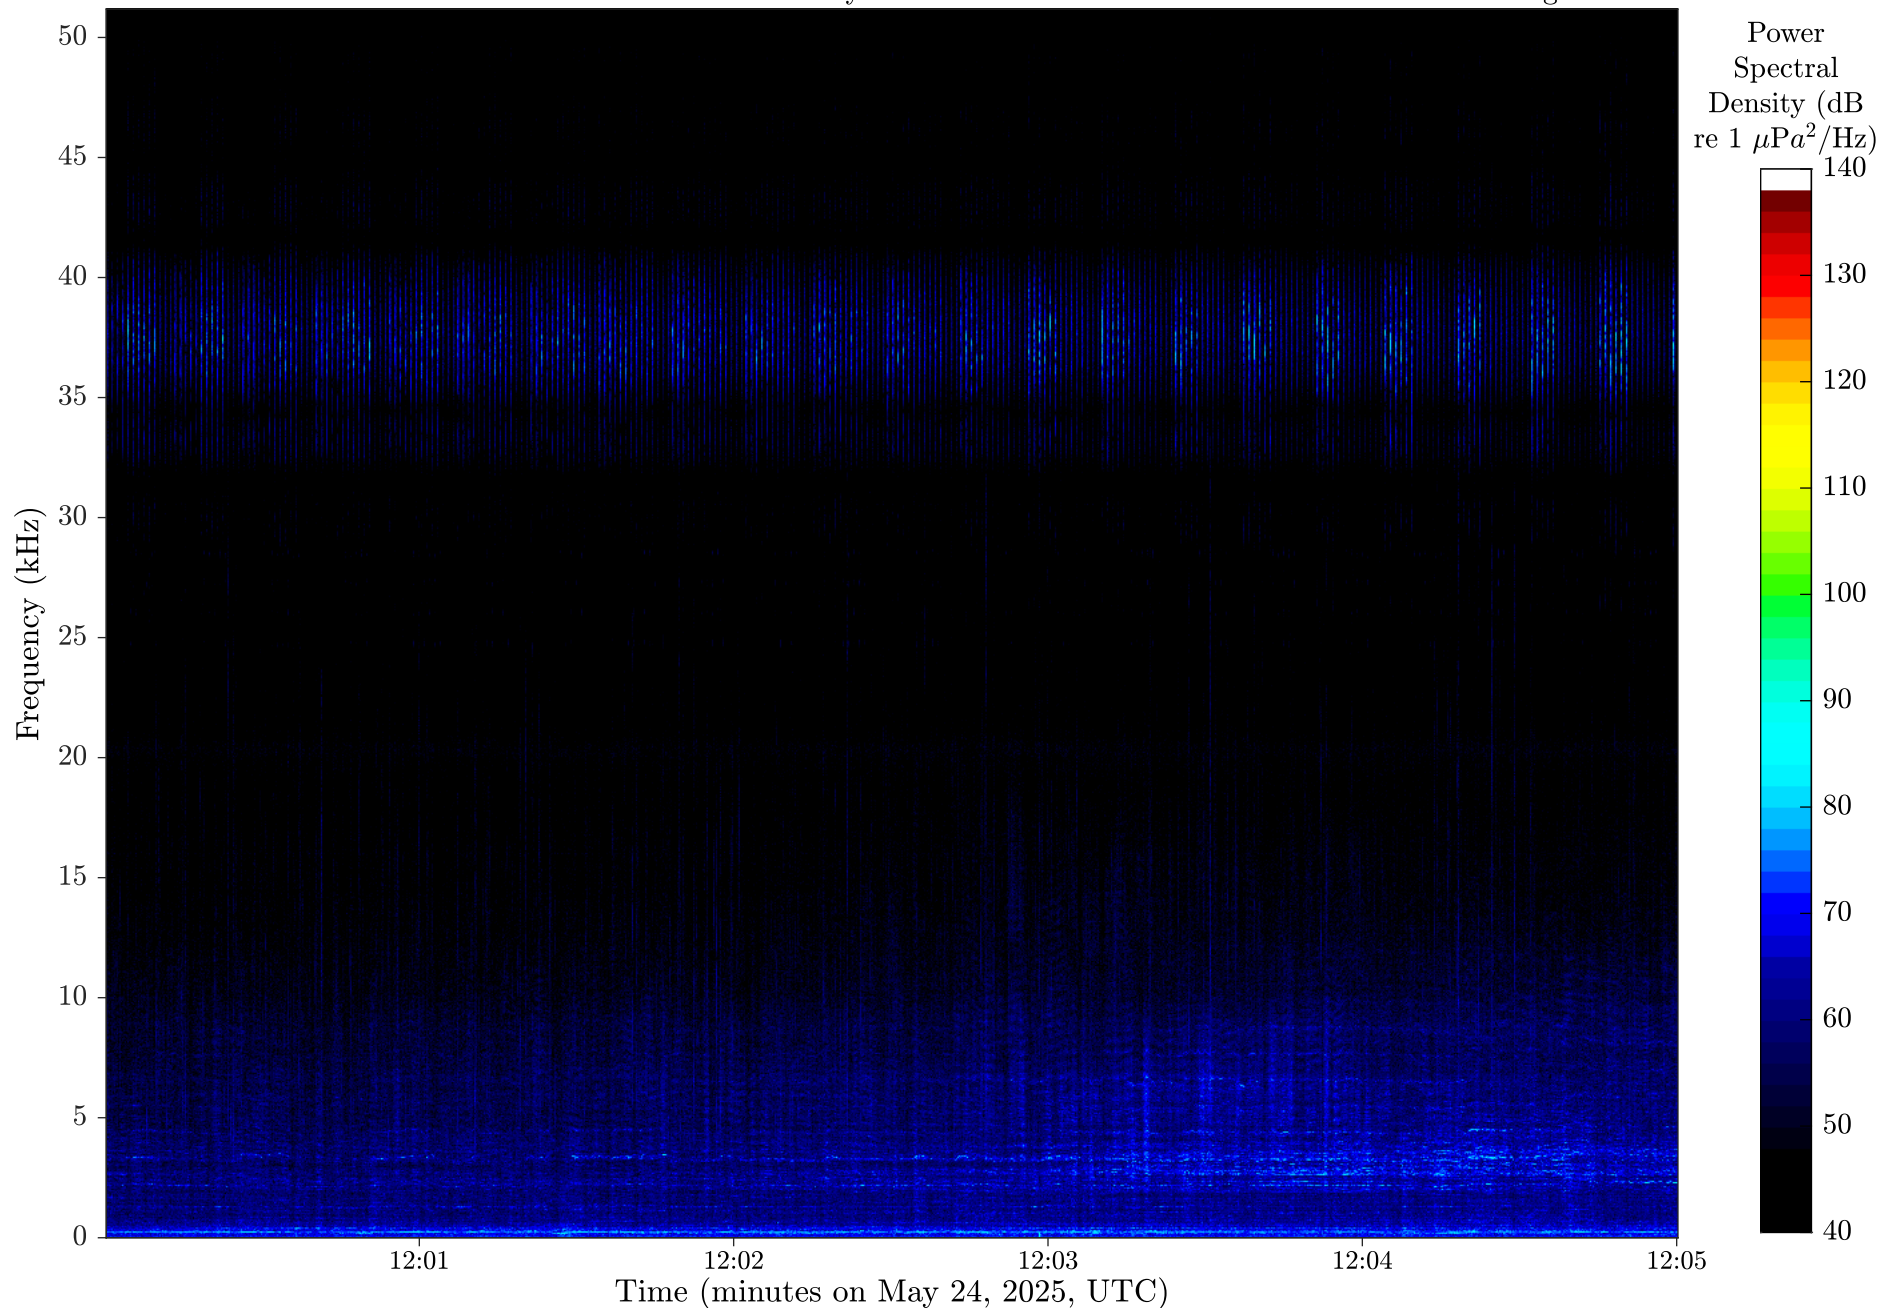

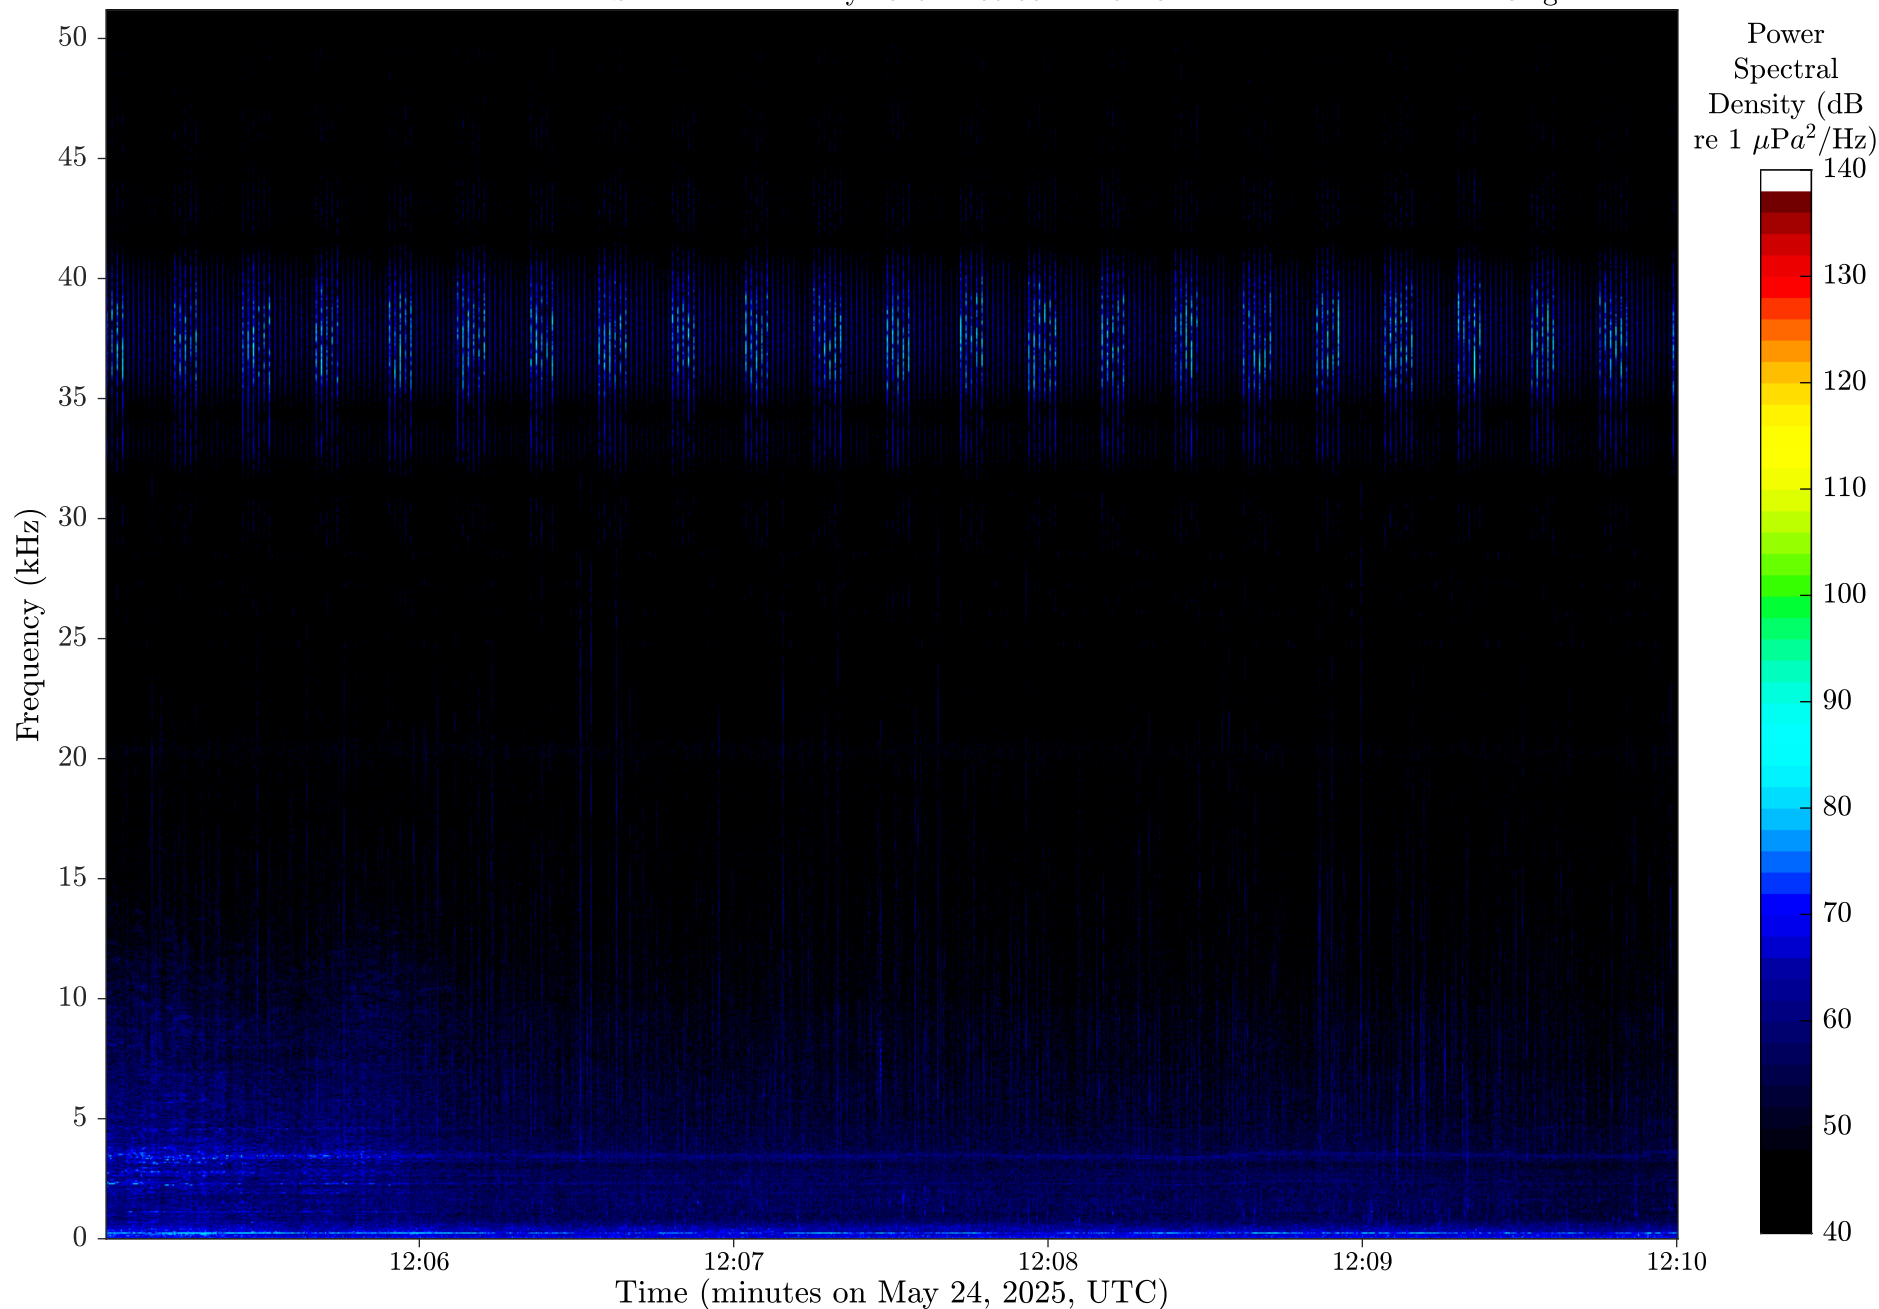


Comments: 29.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:27:16 UTC

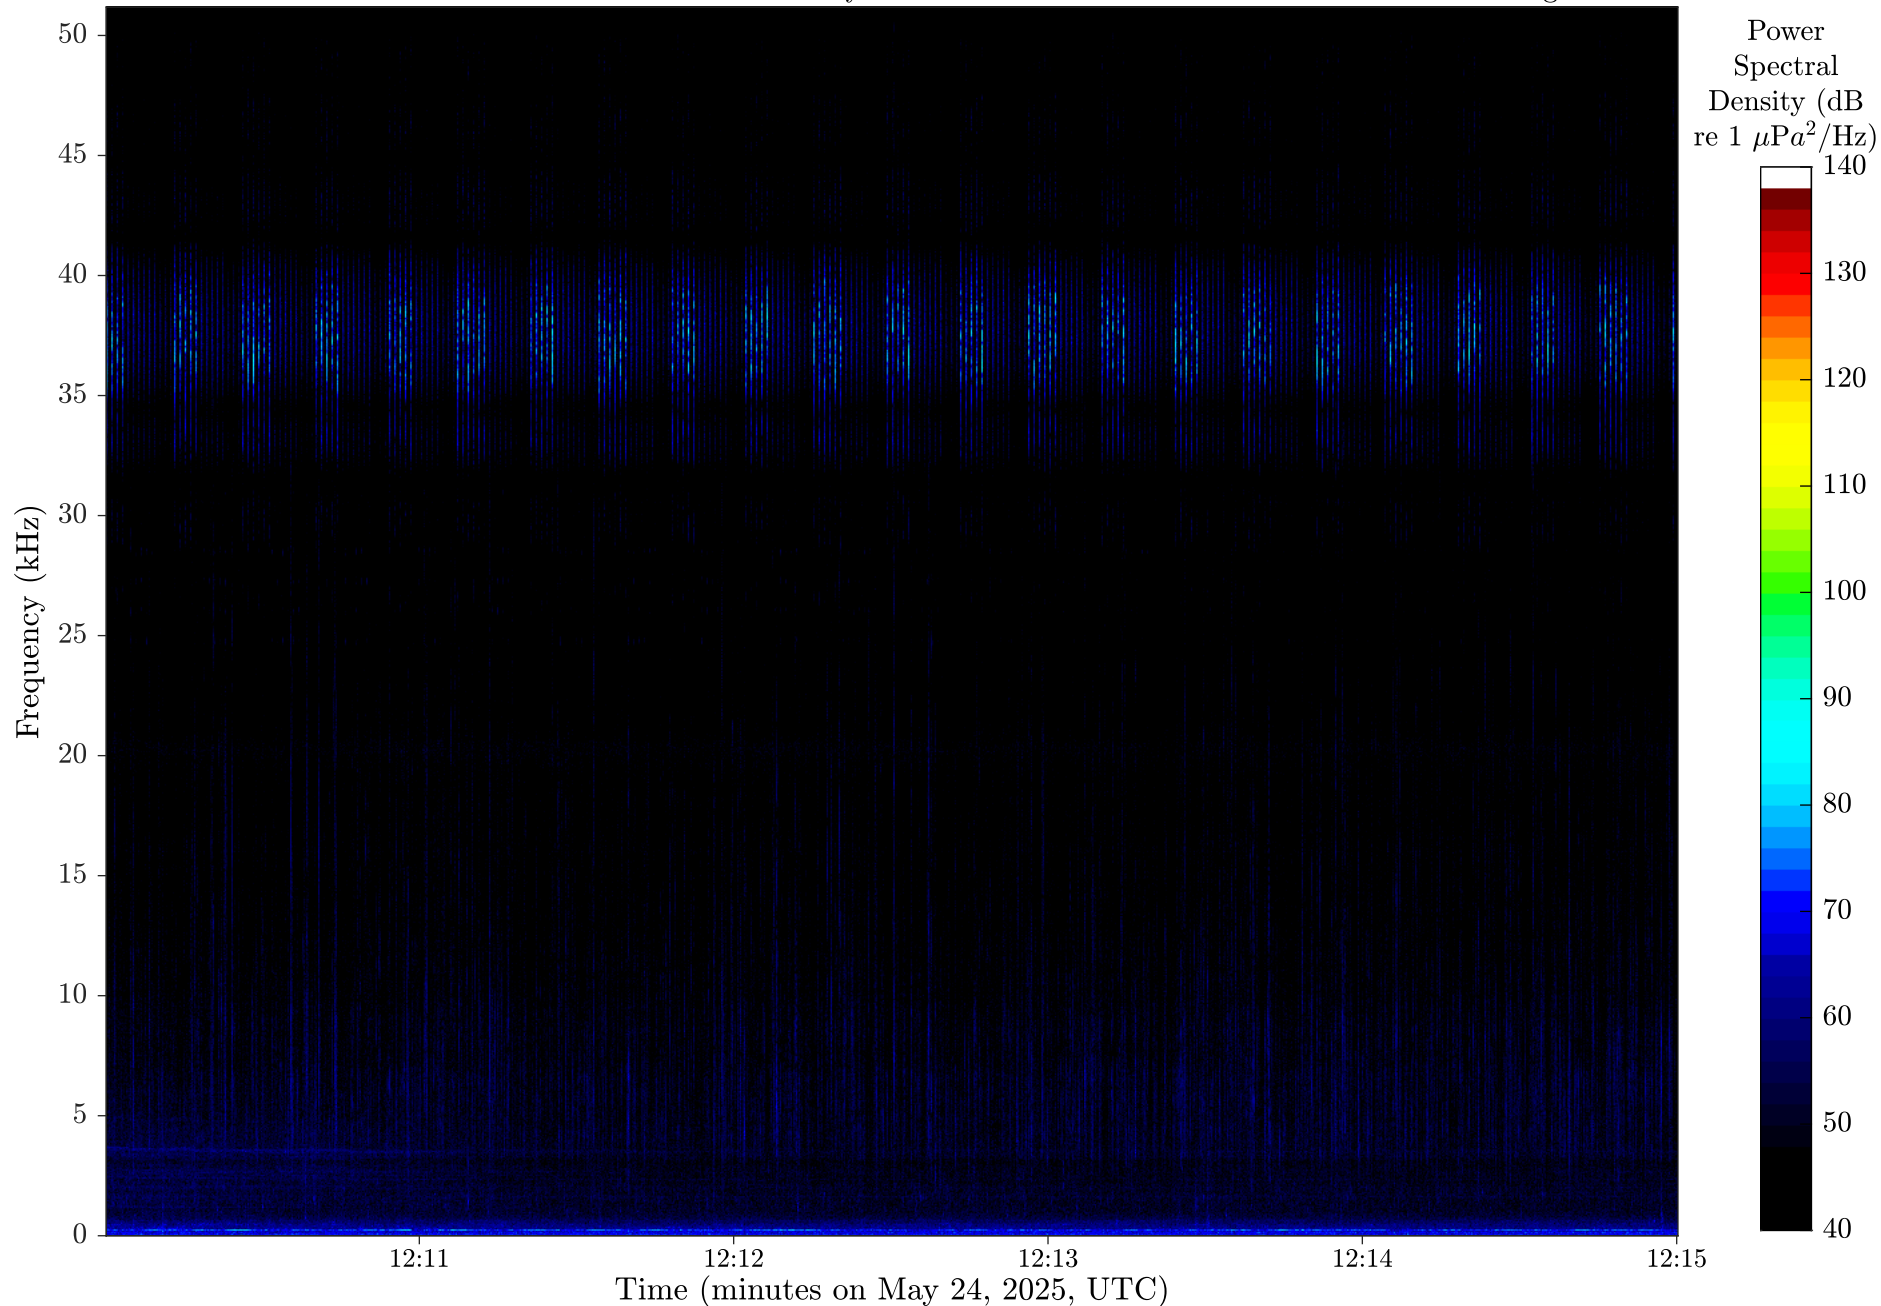

Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:27:24 UTC

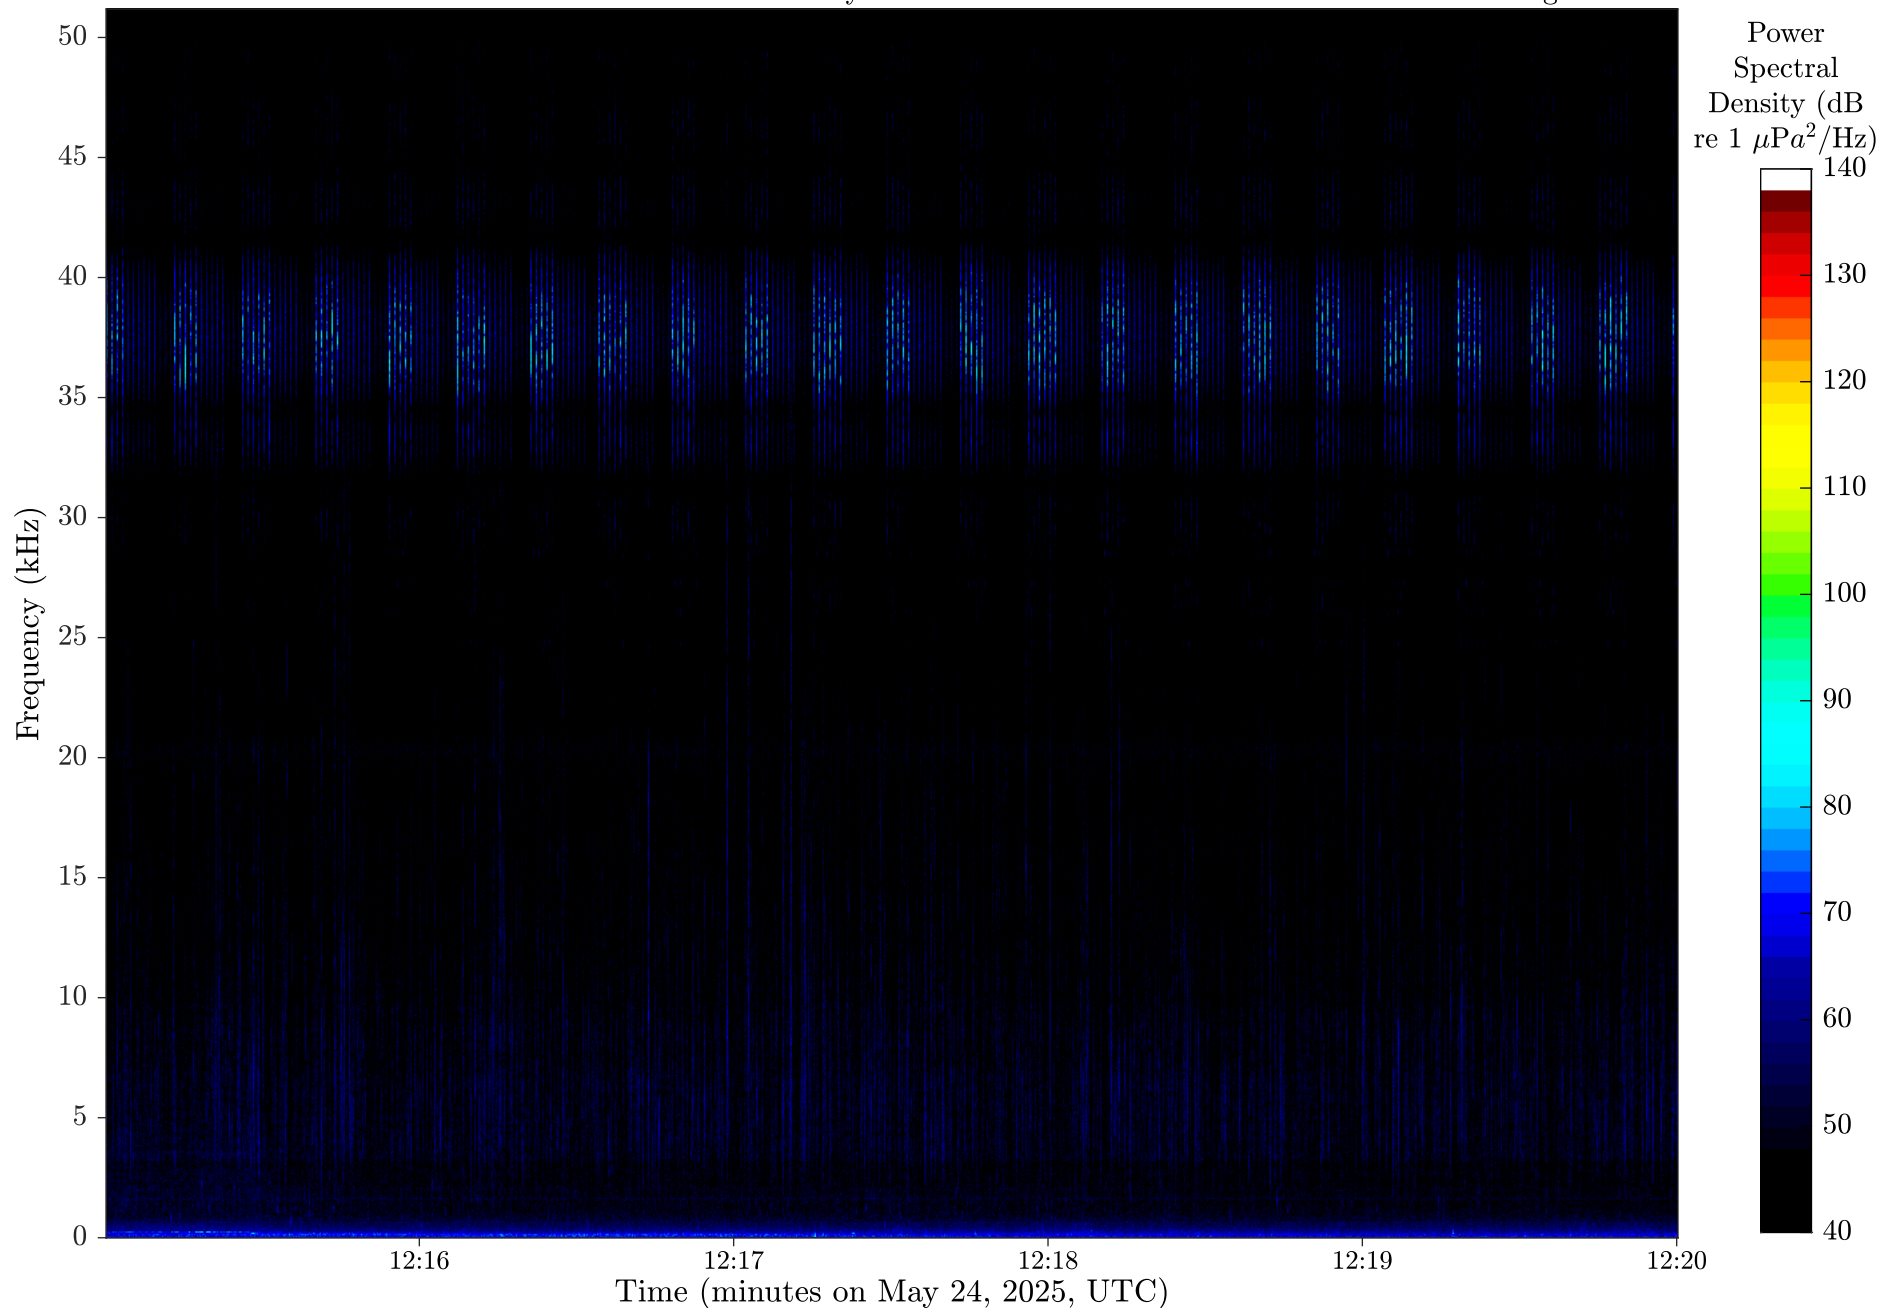

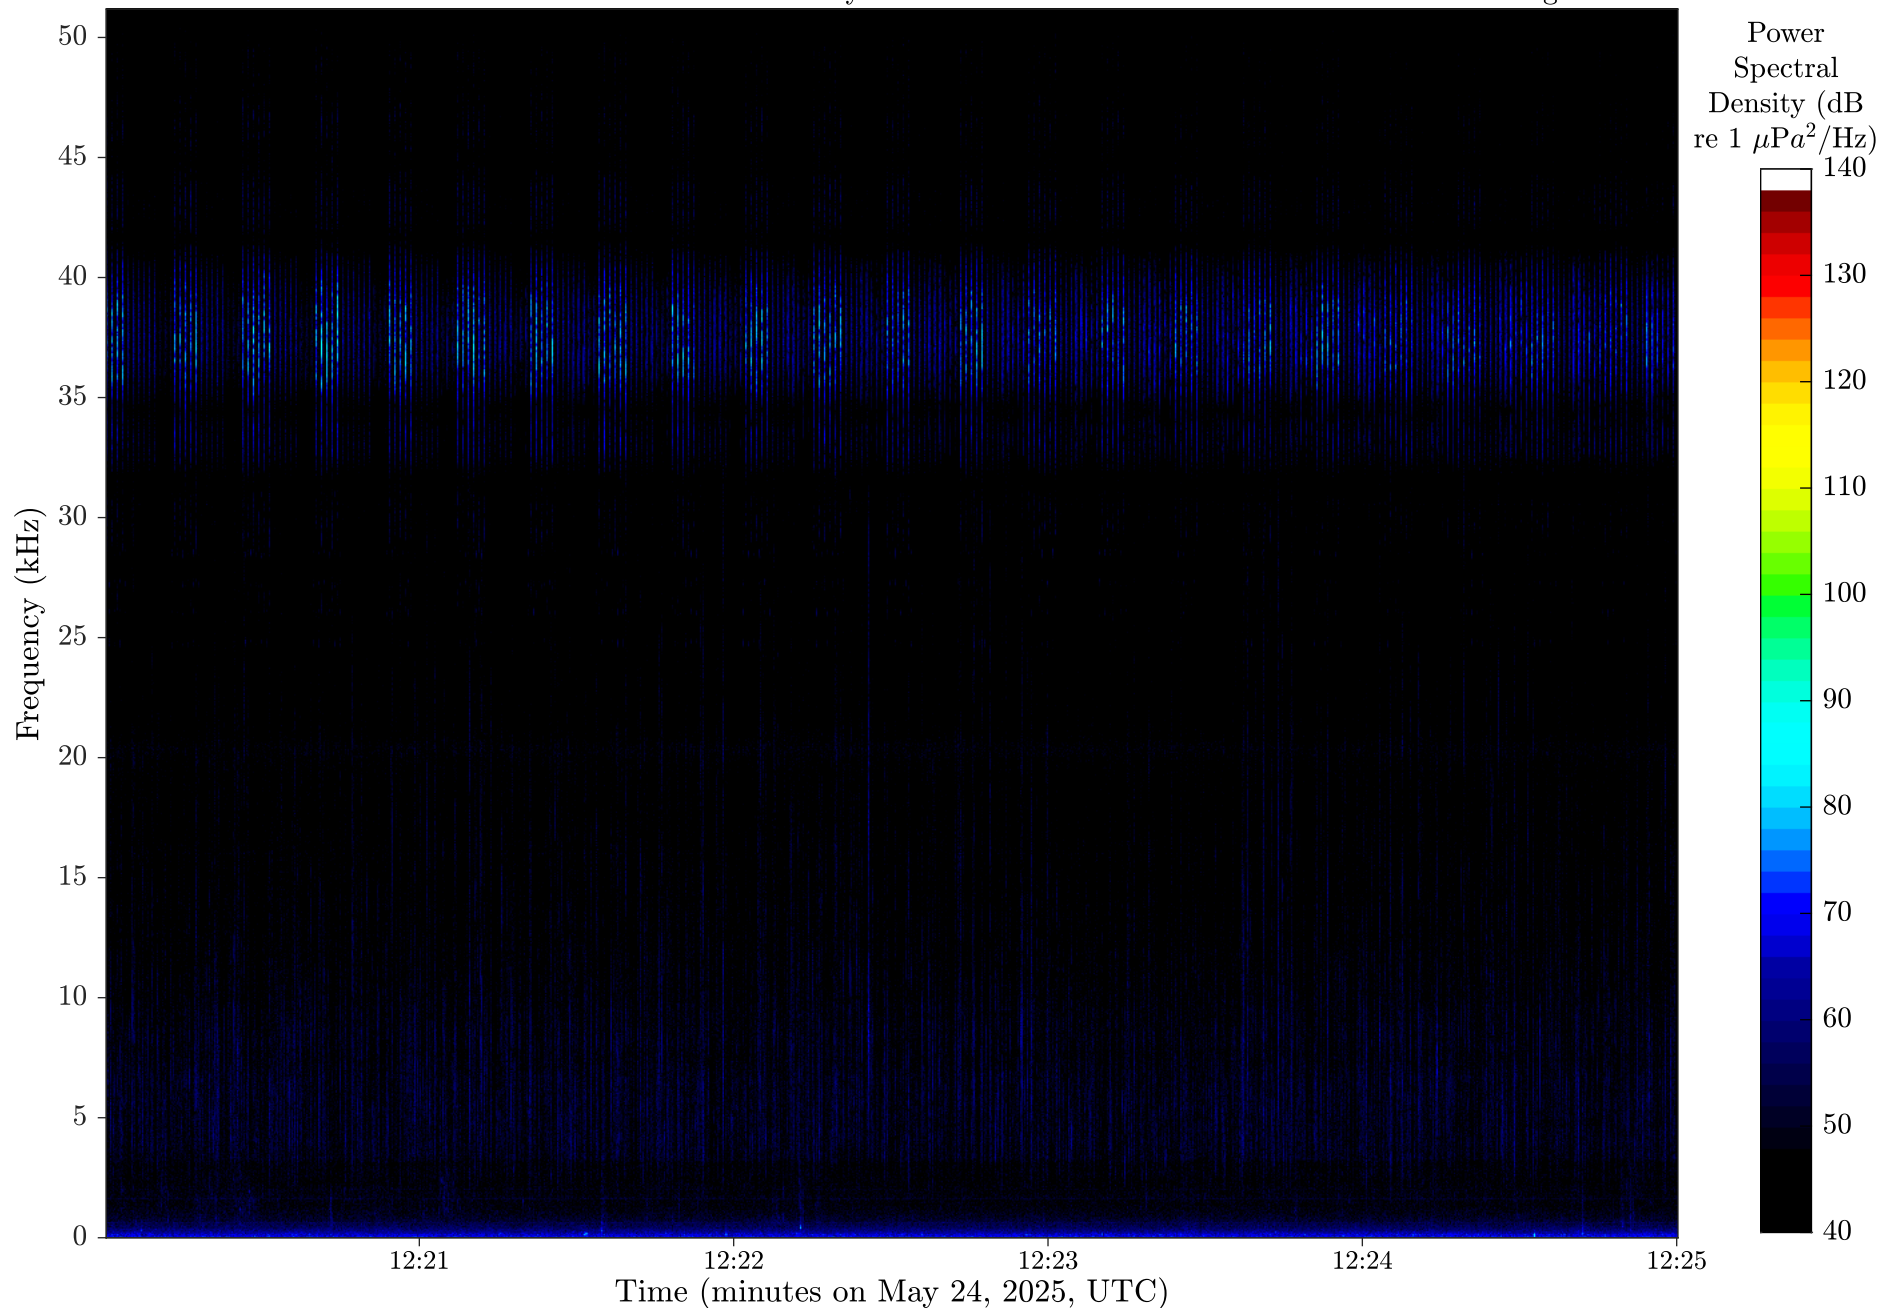


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:27:39 UTC

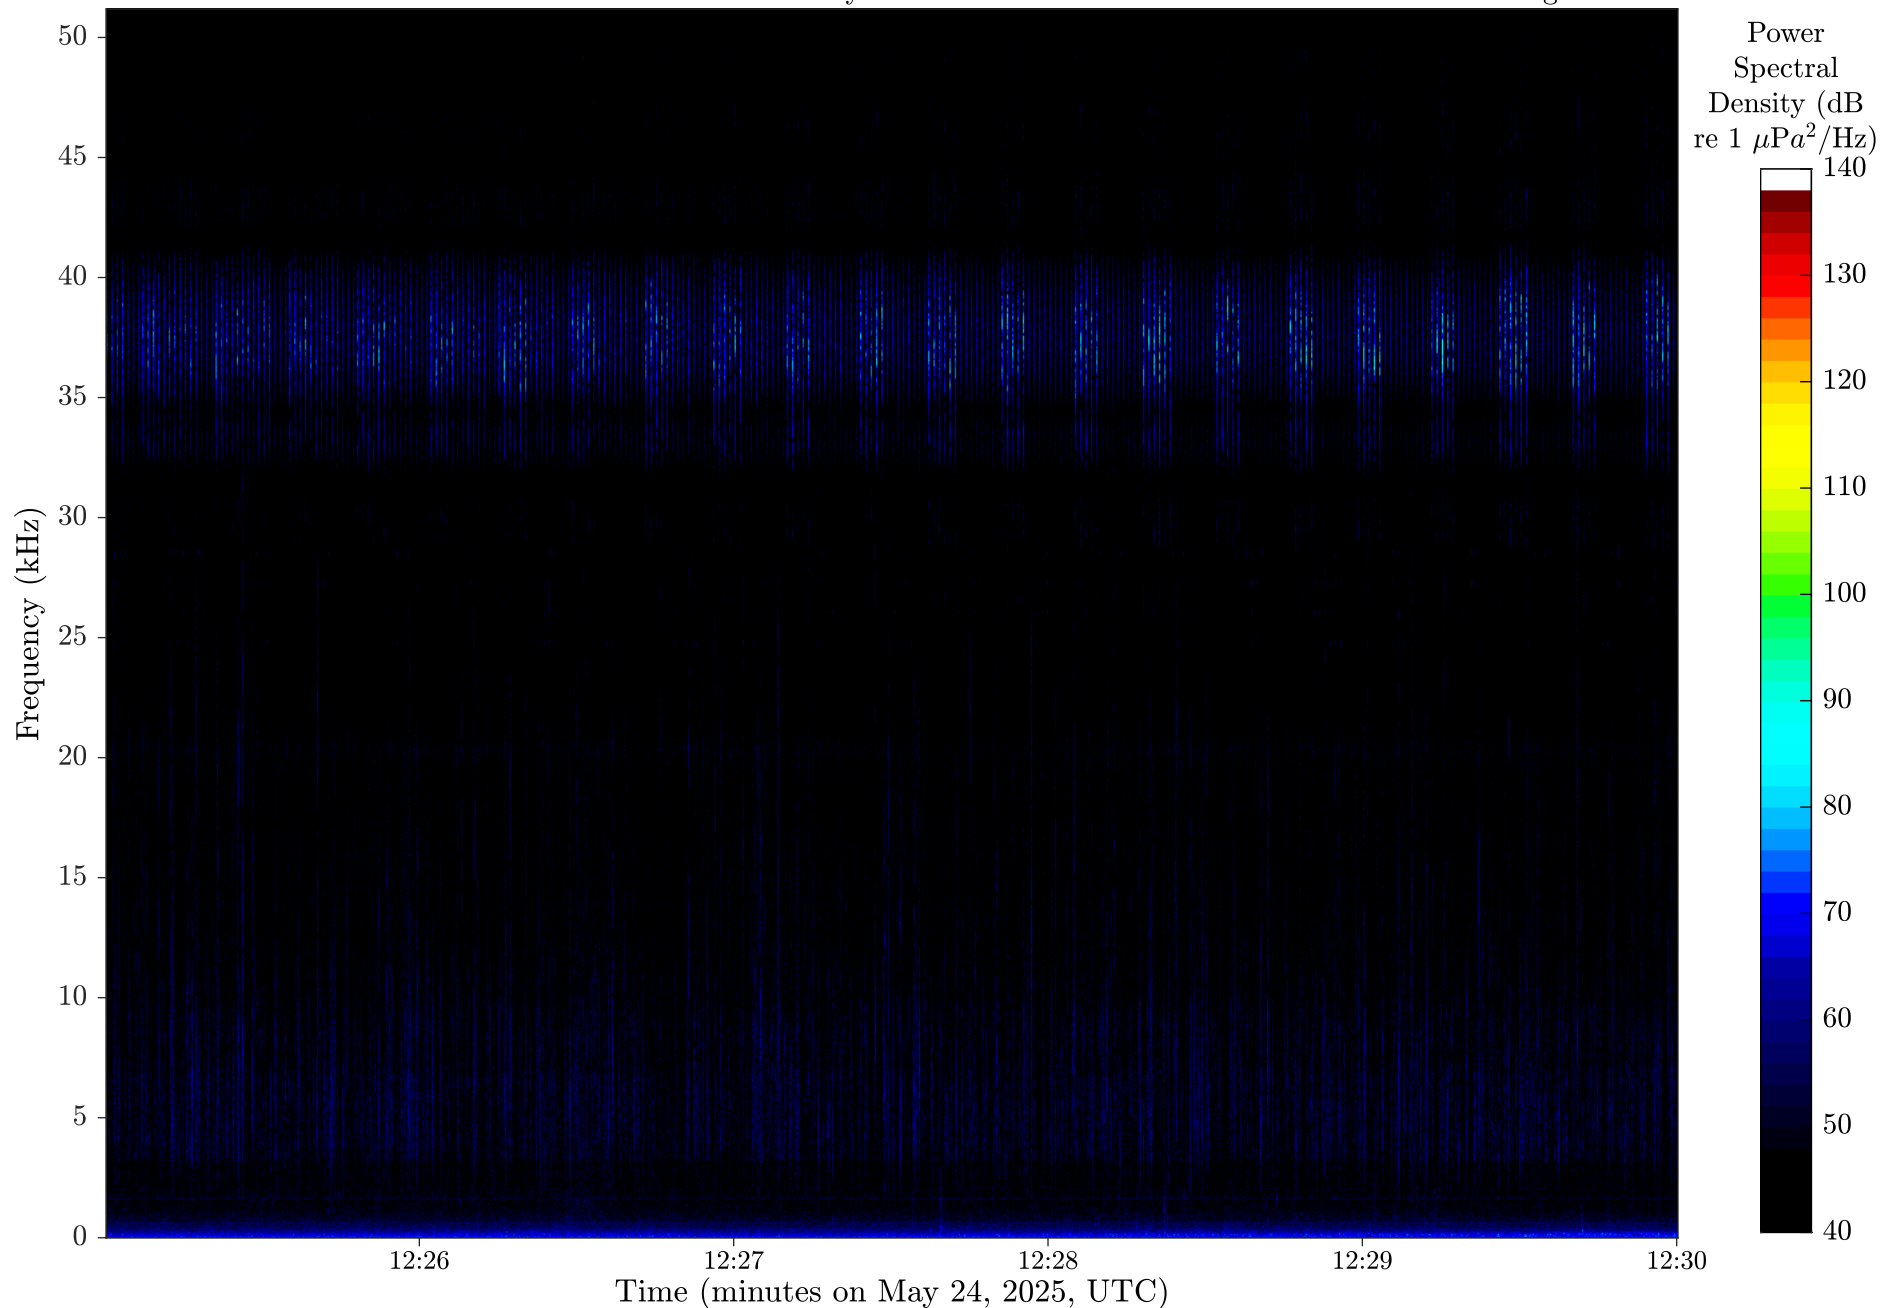


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:27:47 UTC

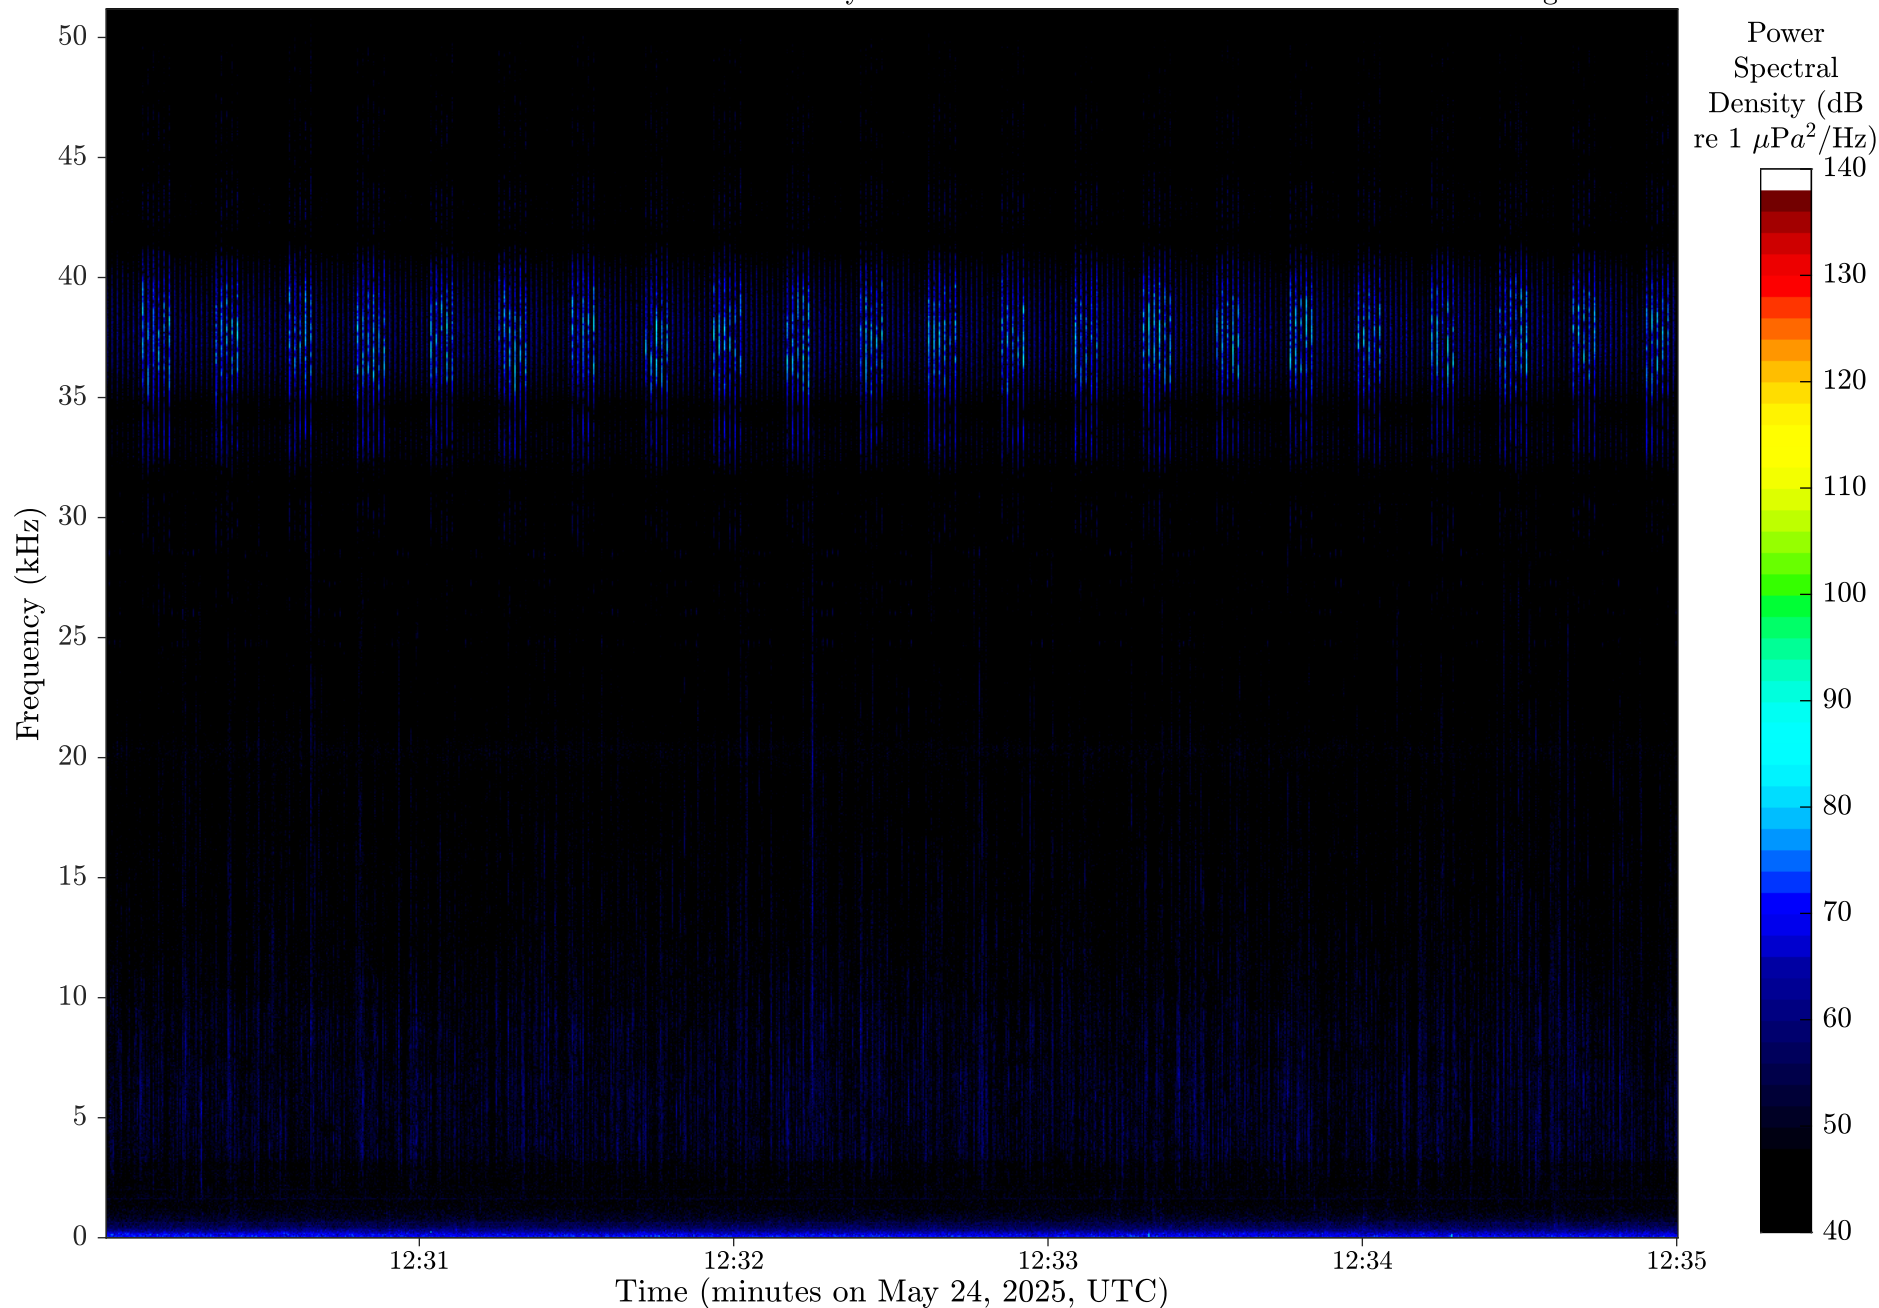


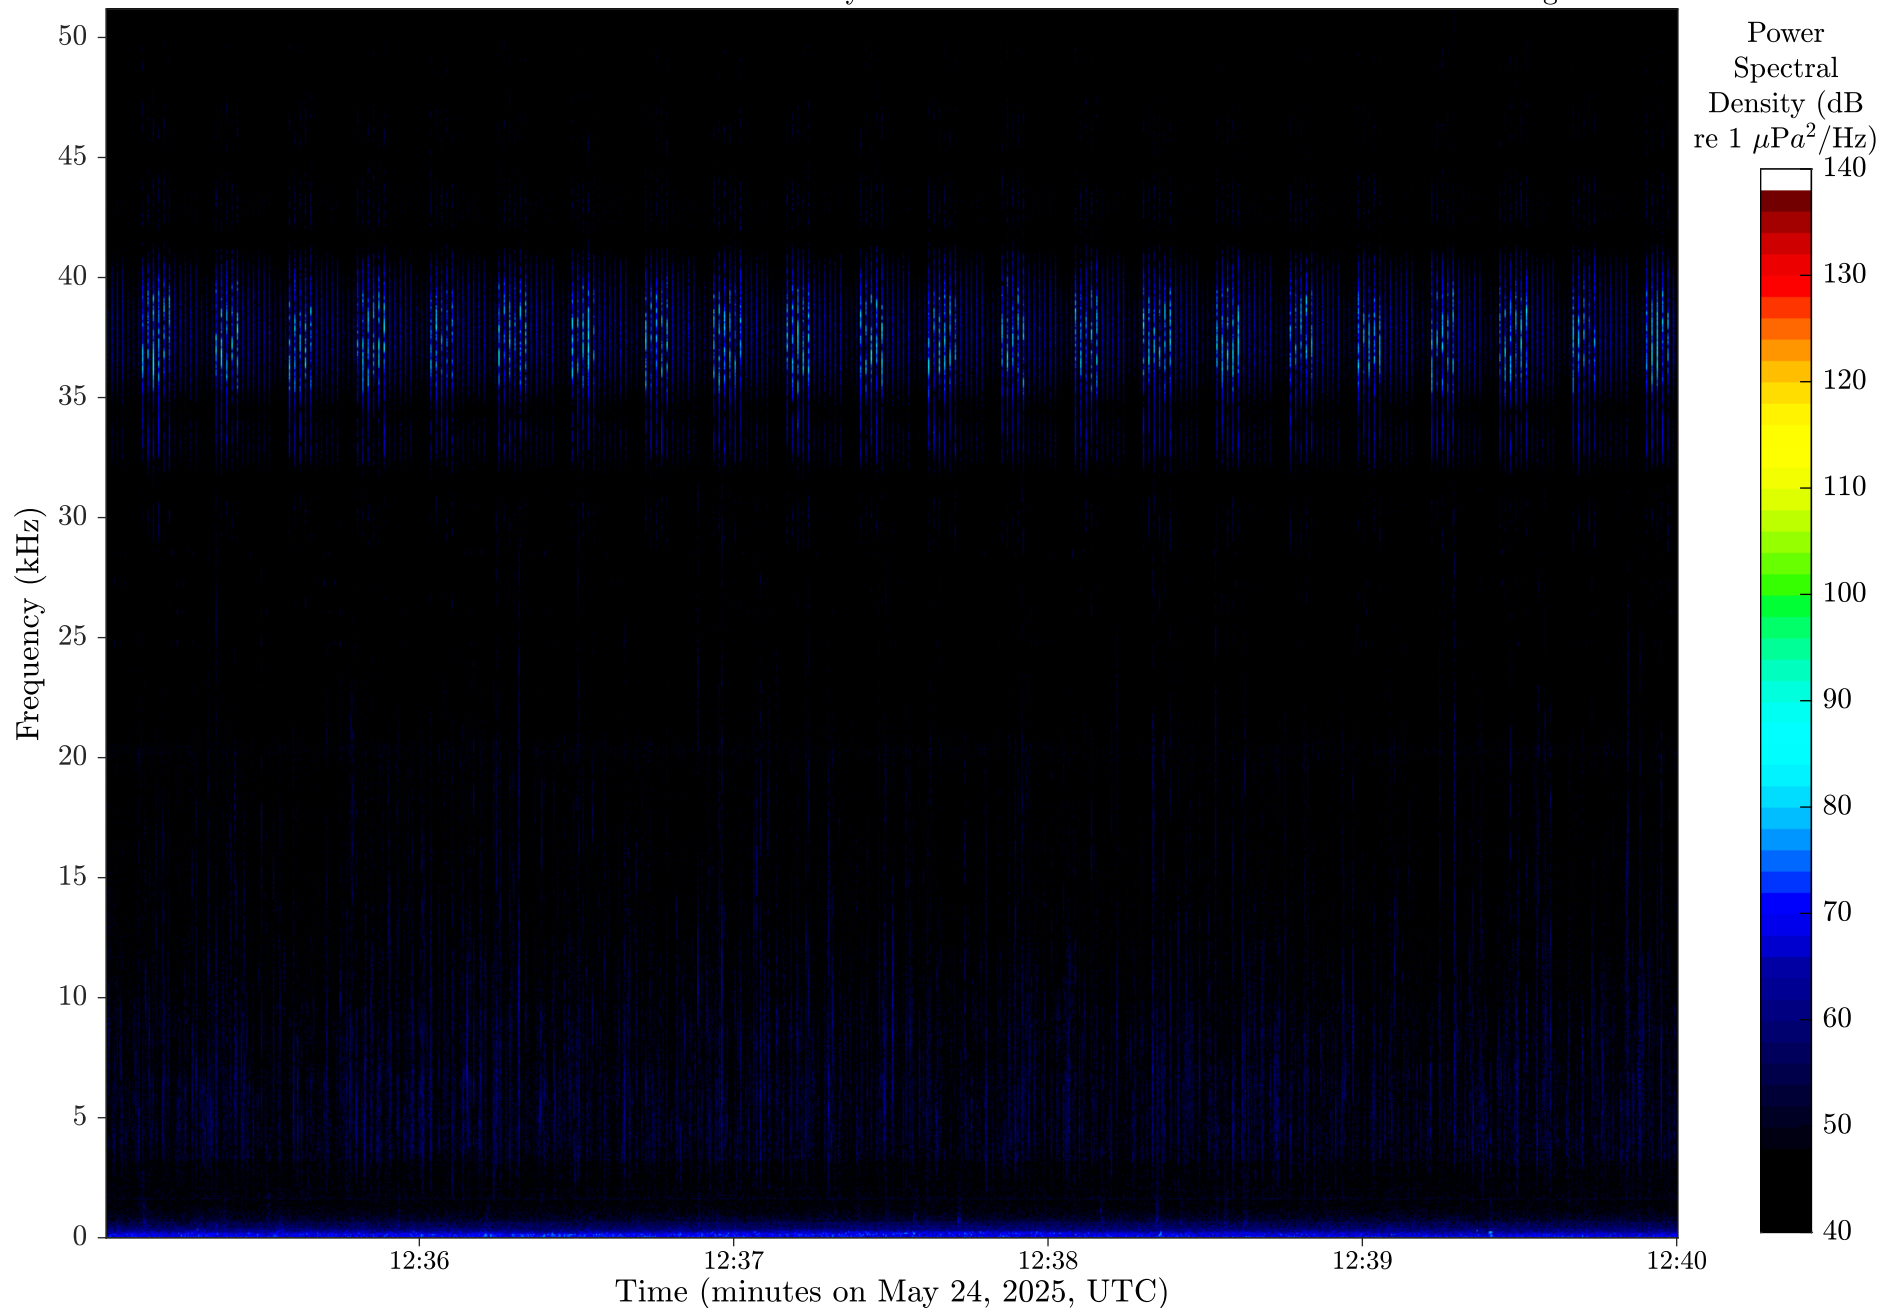


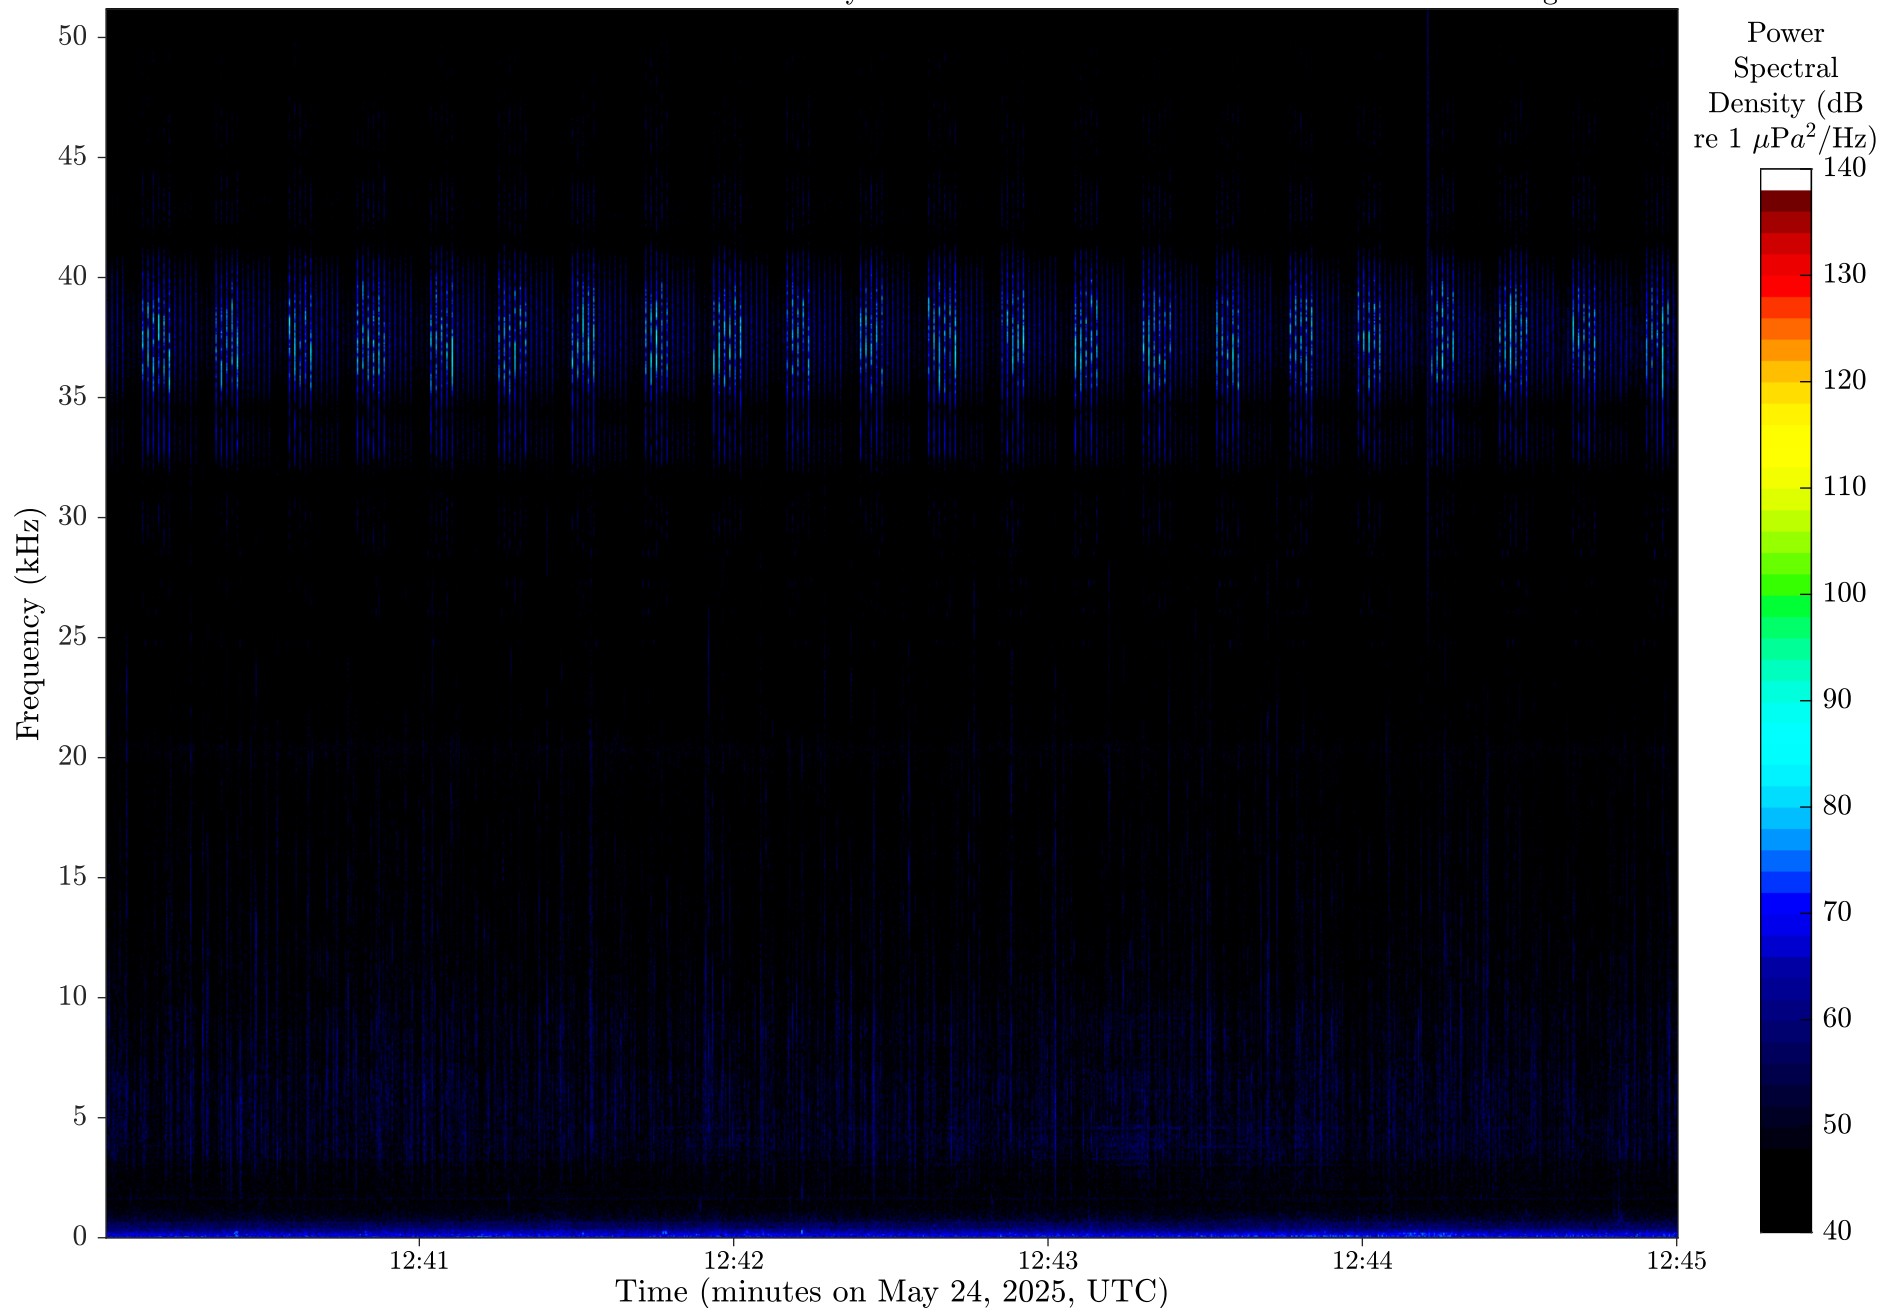


Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:28:10 UTC

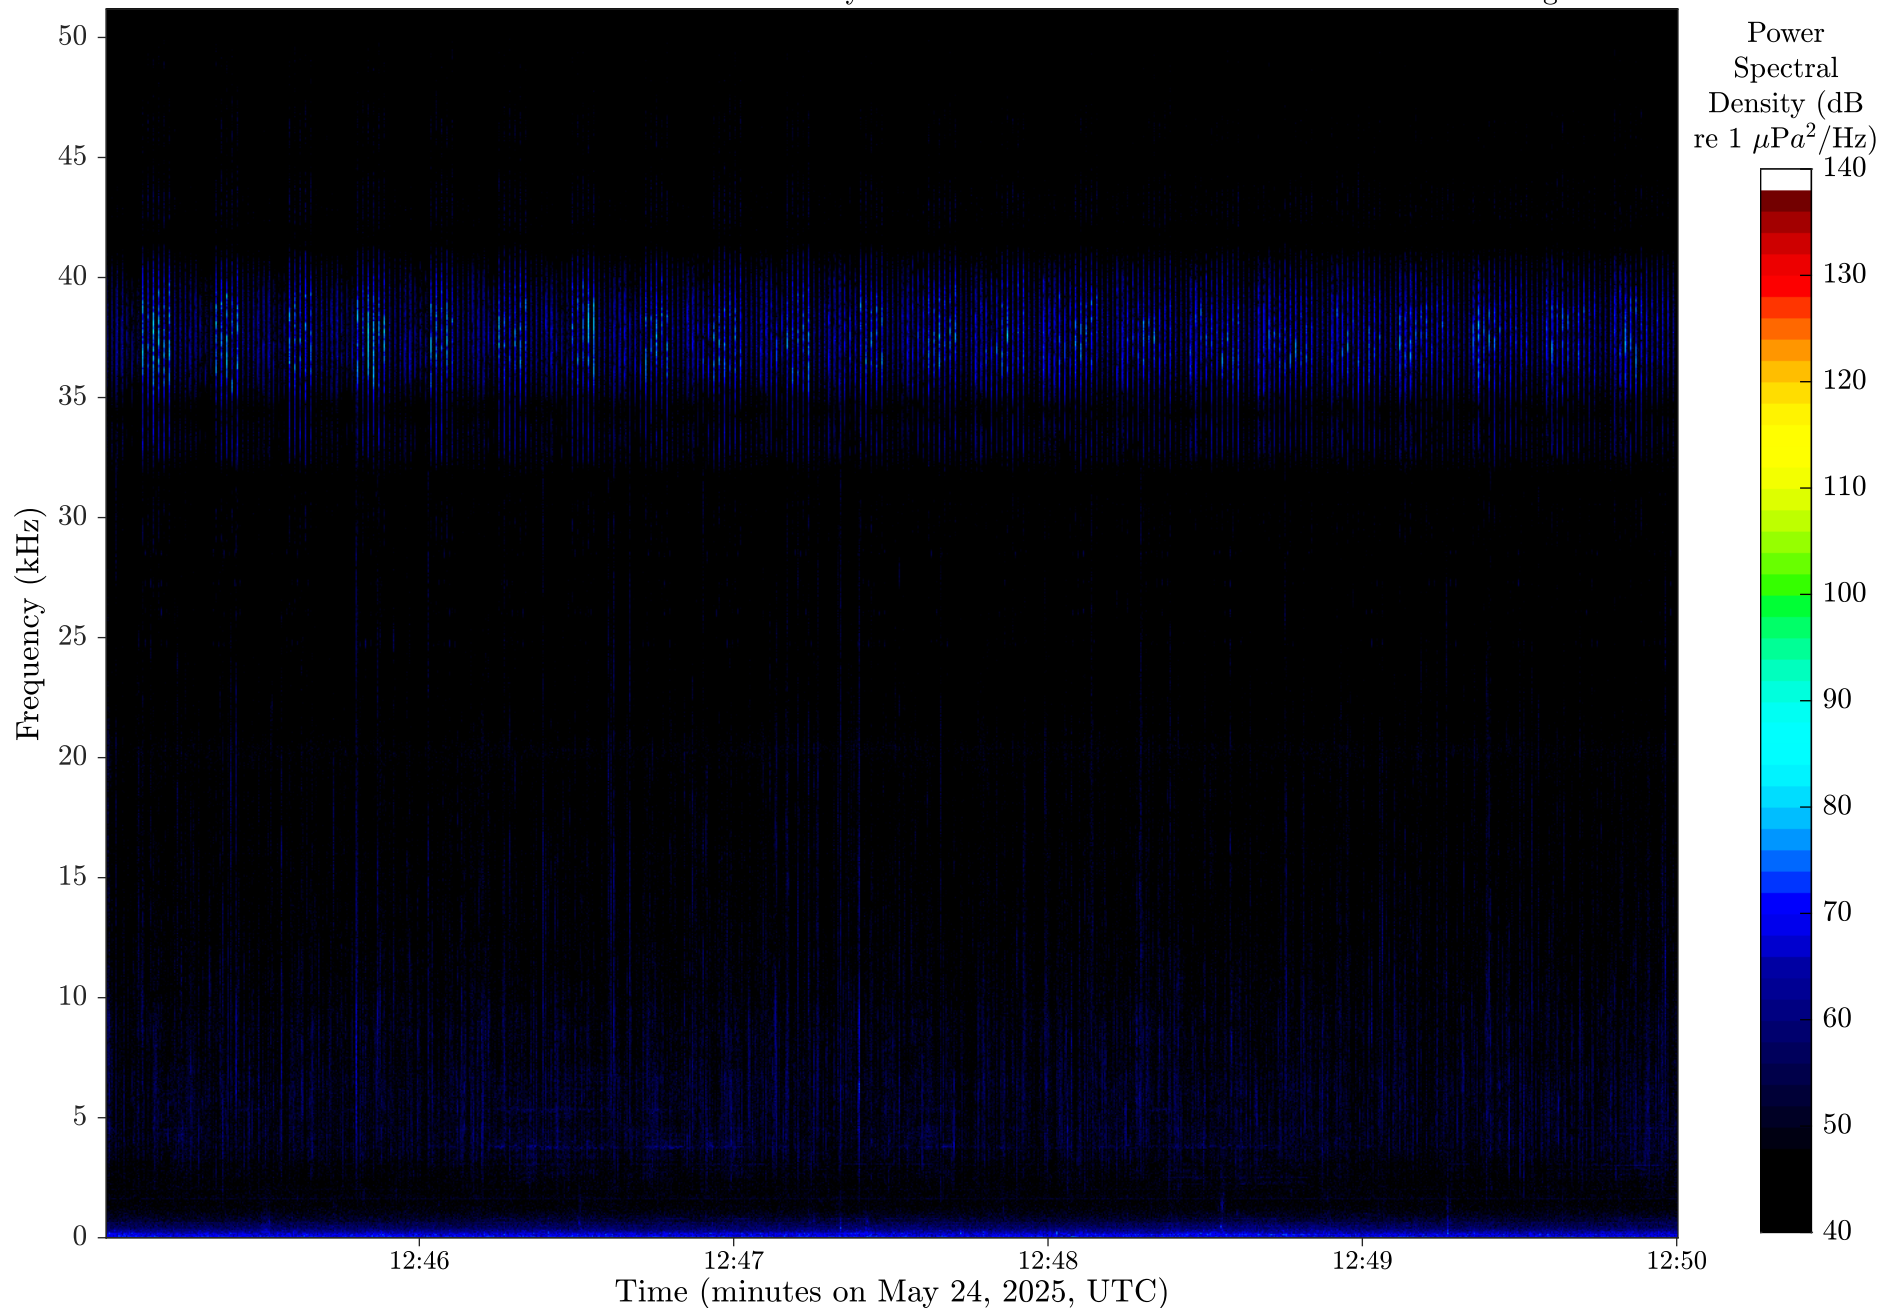


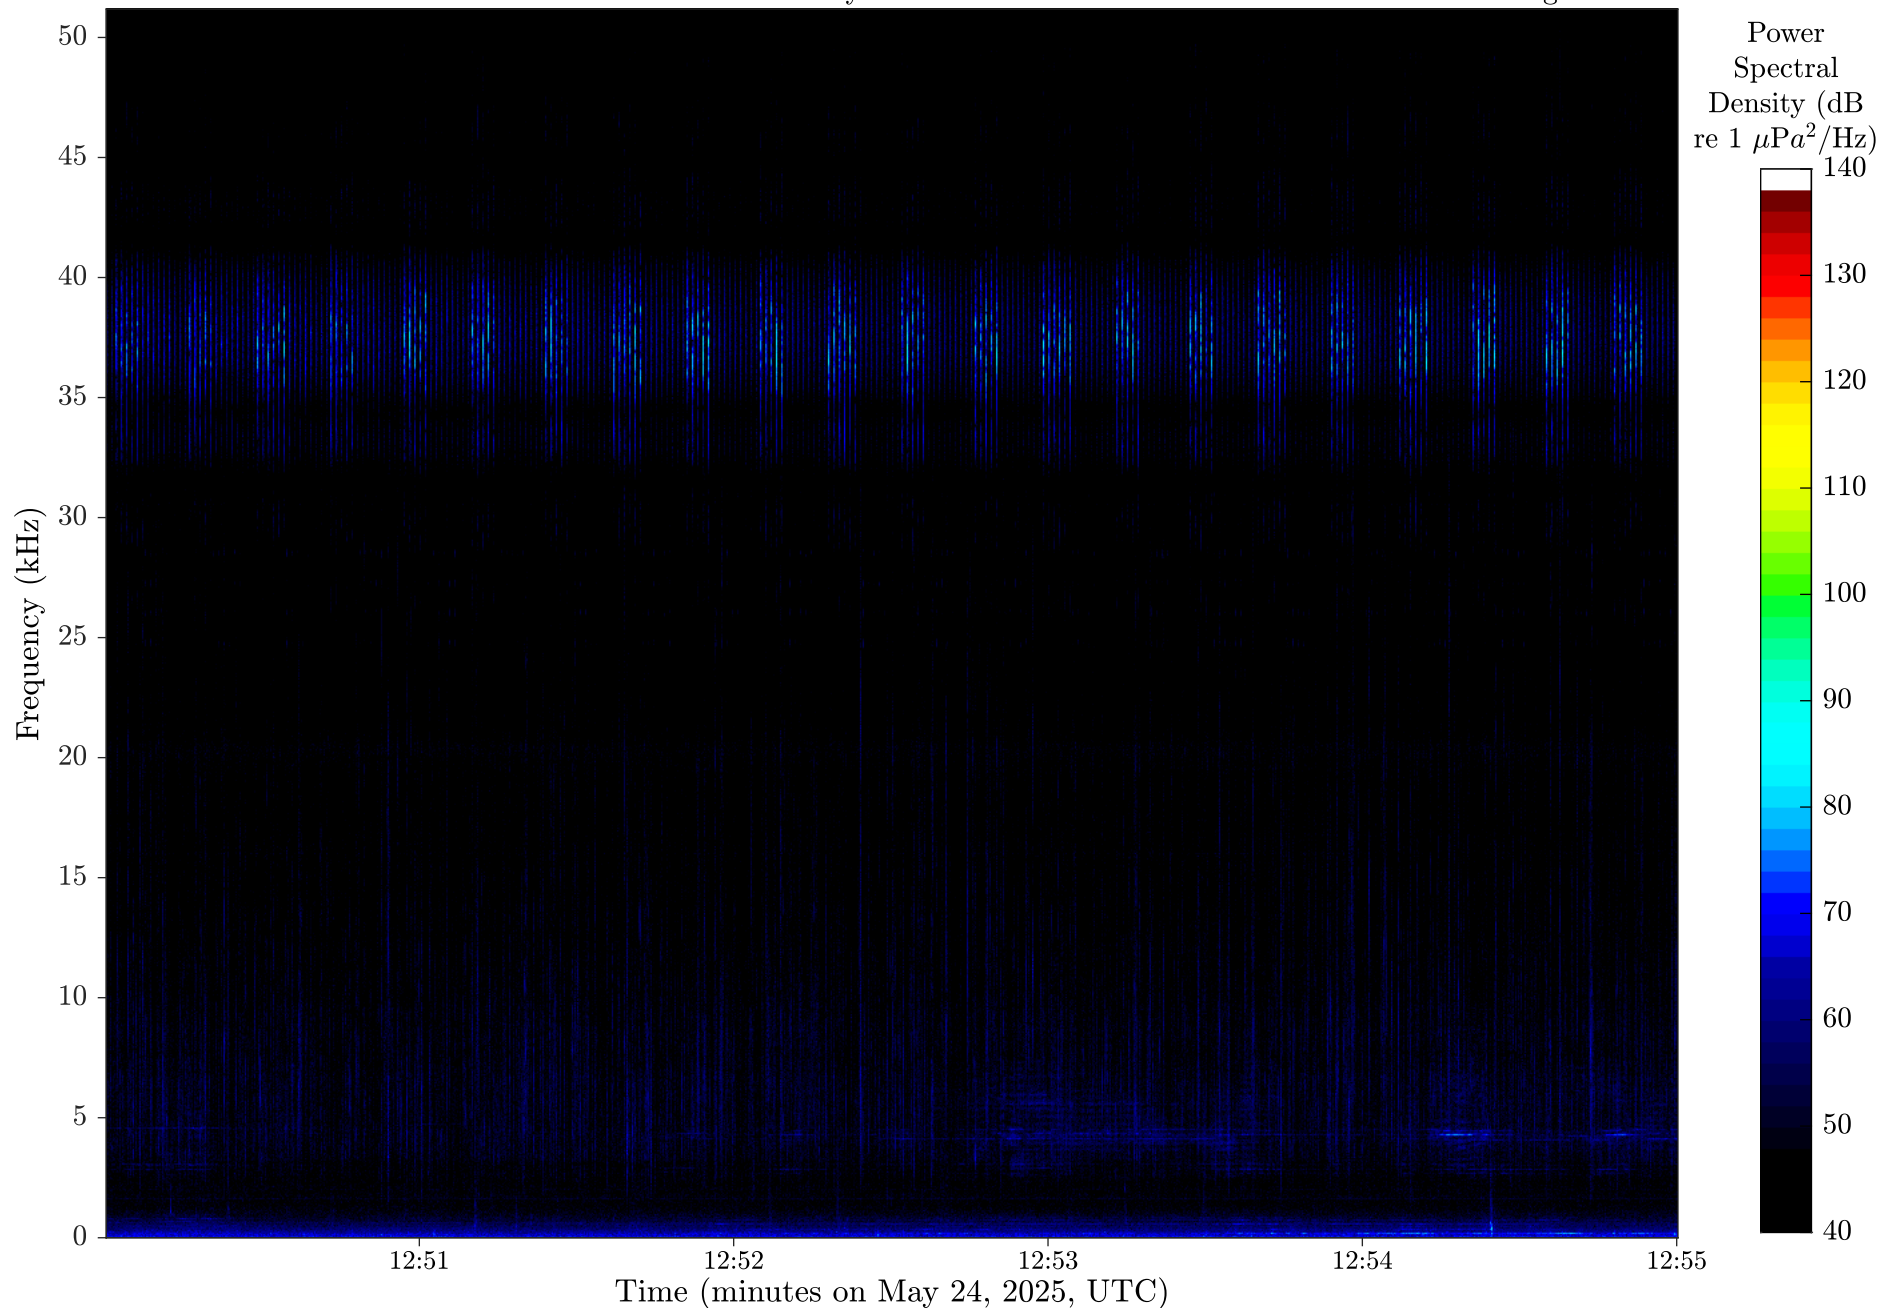


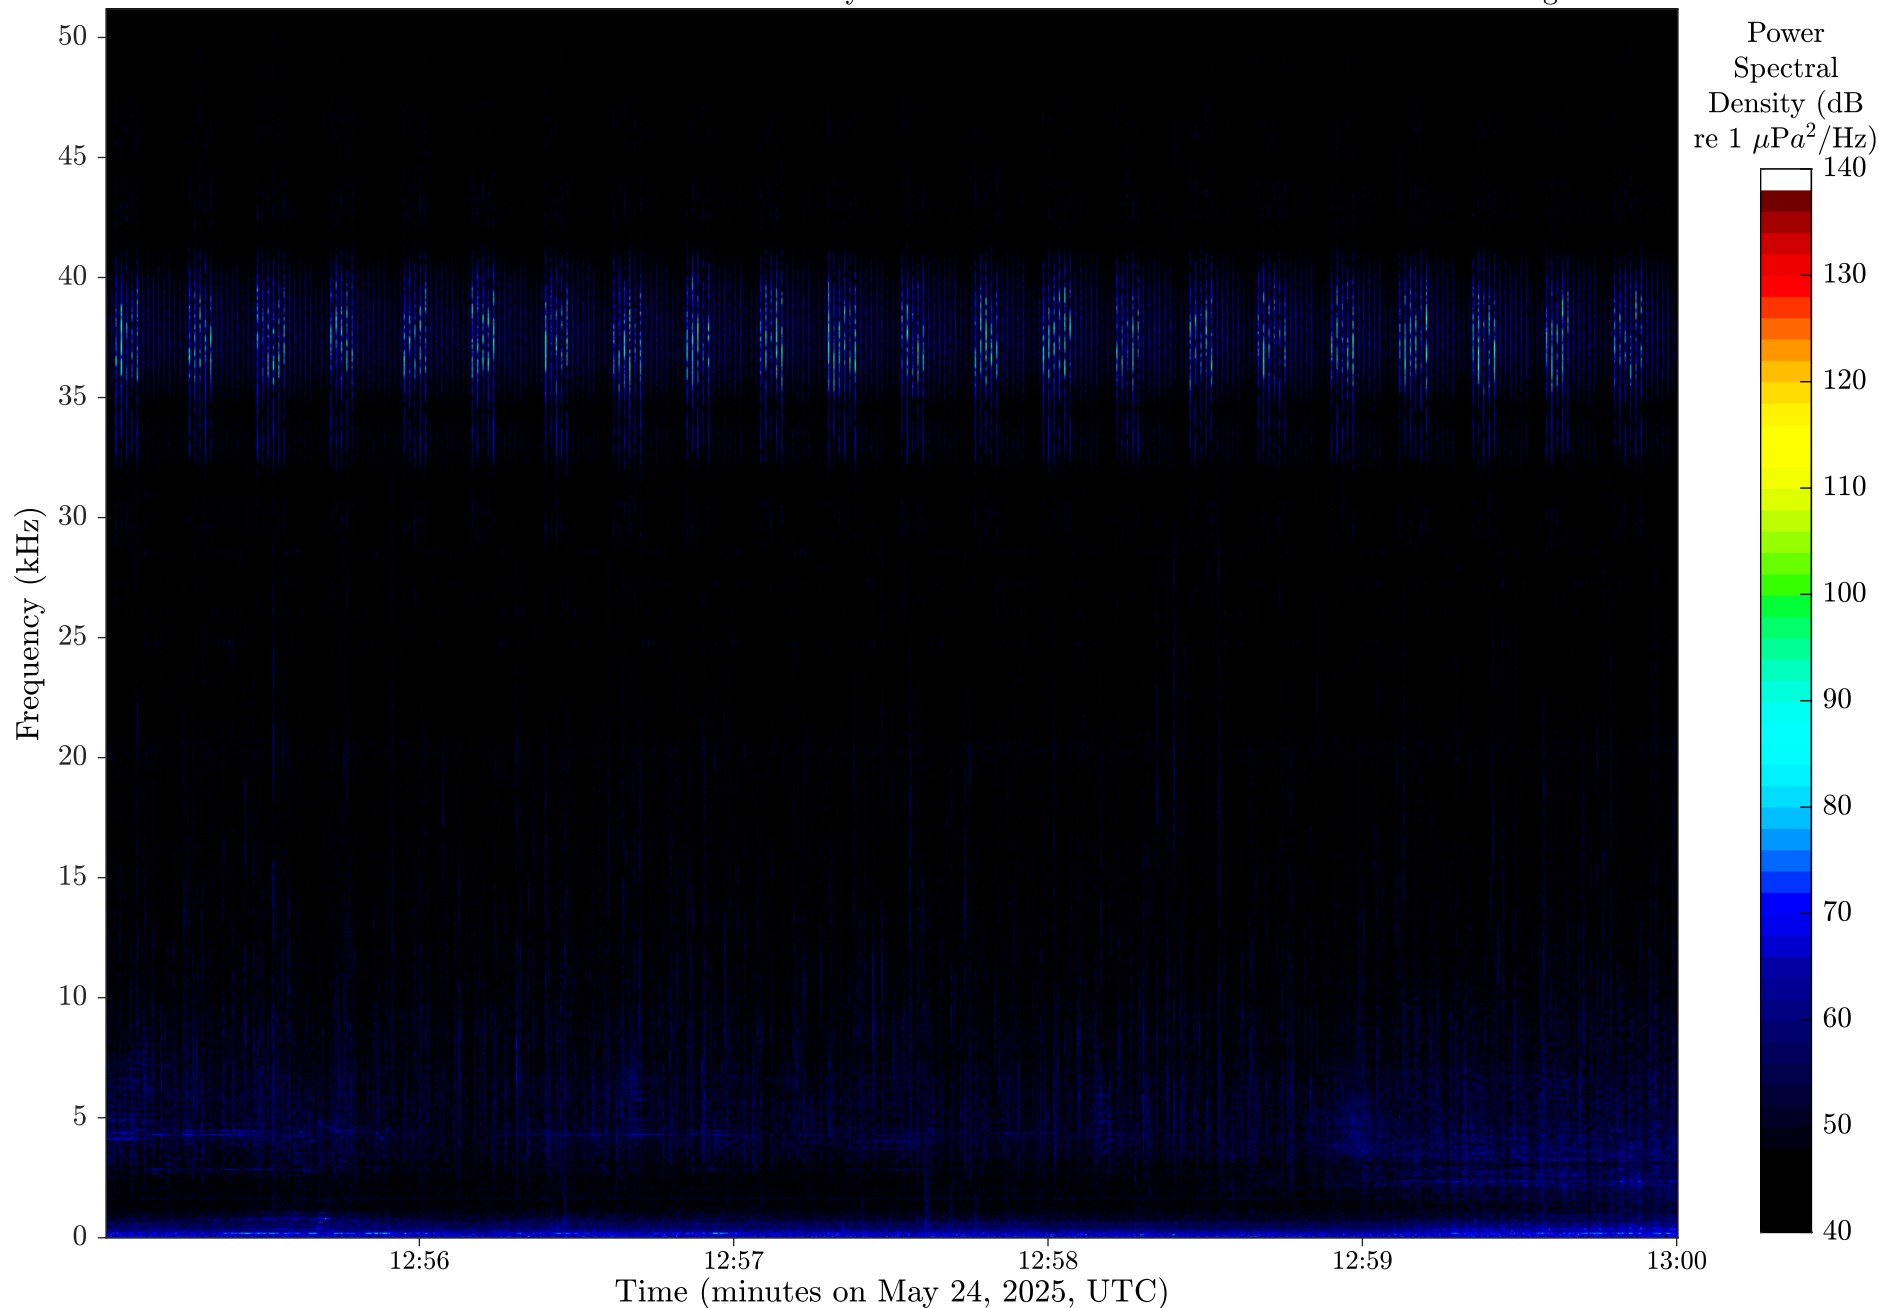

Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:28:34 UTC

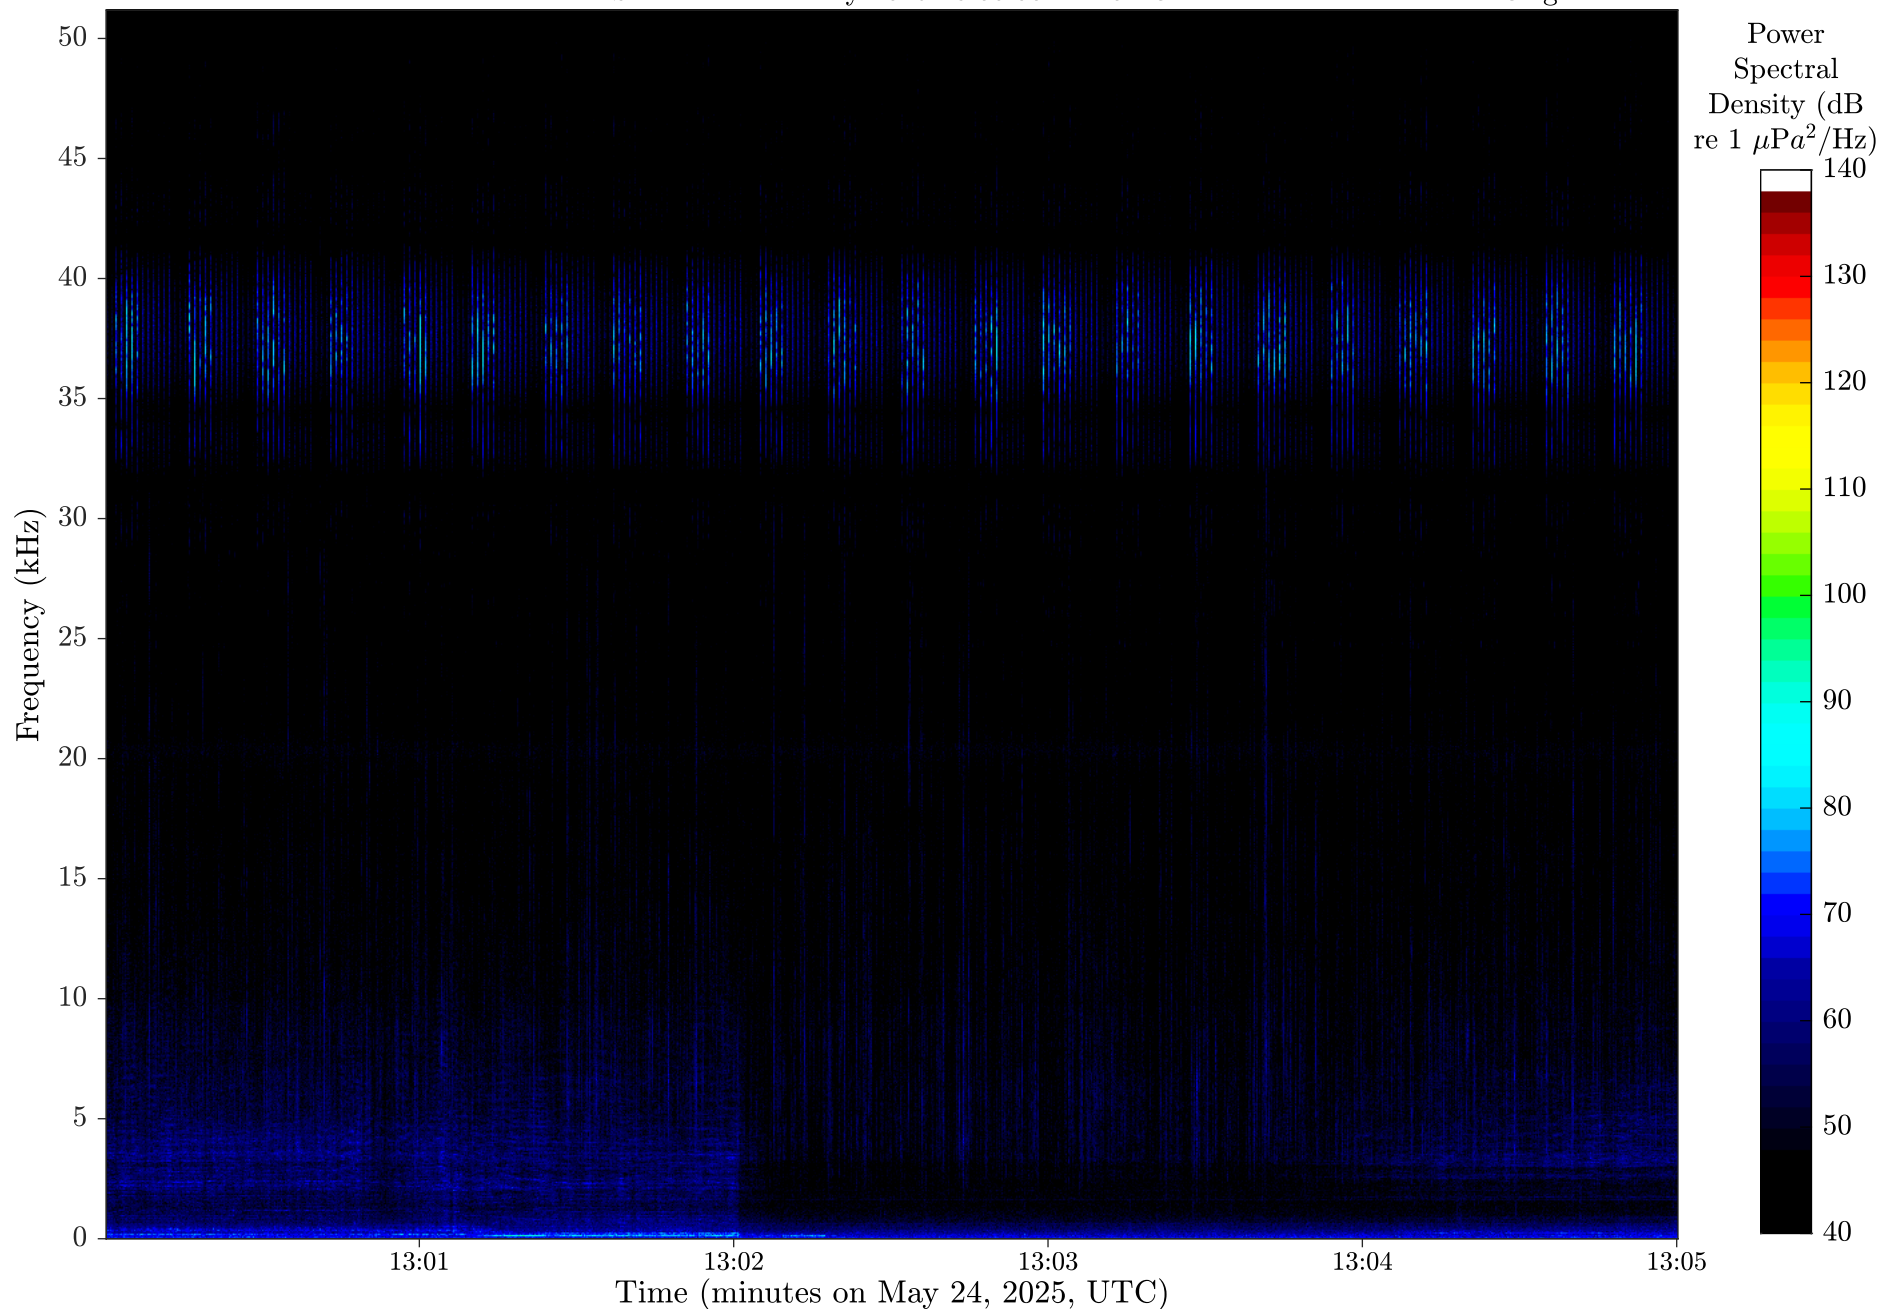


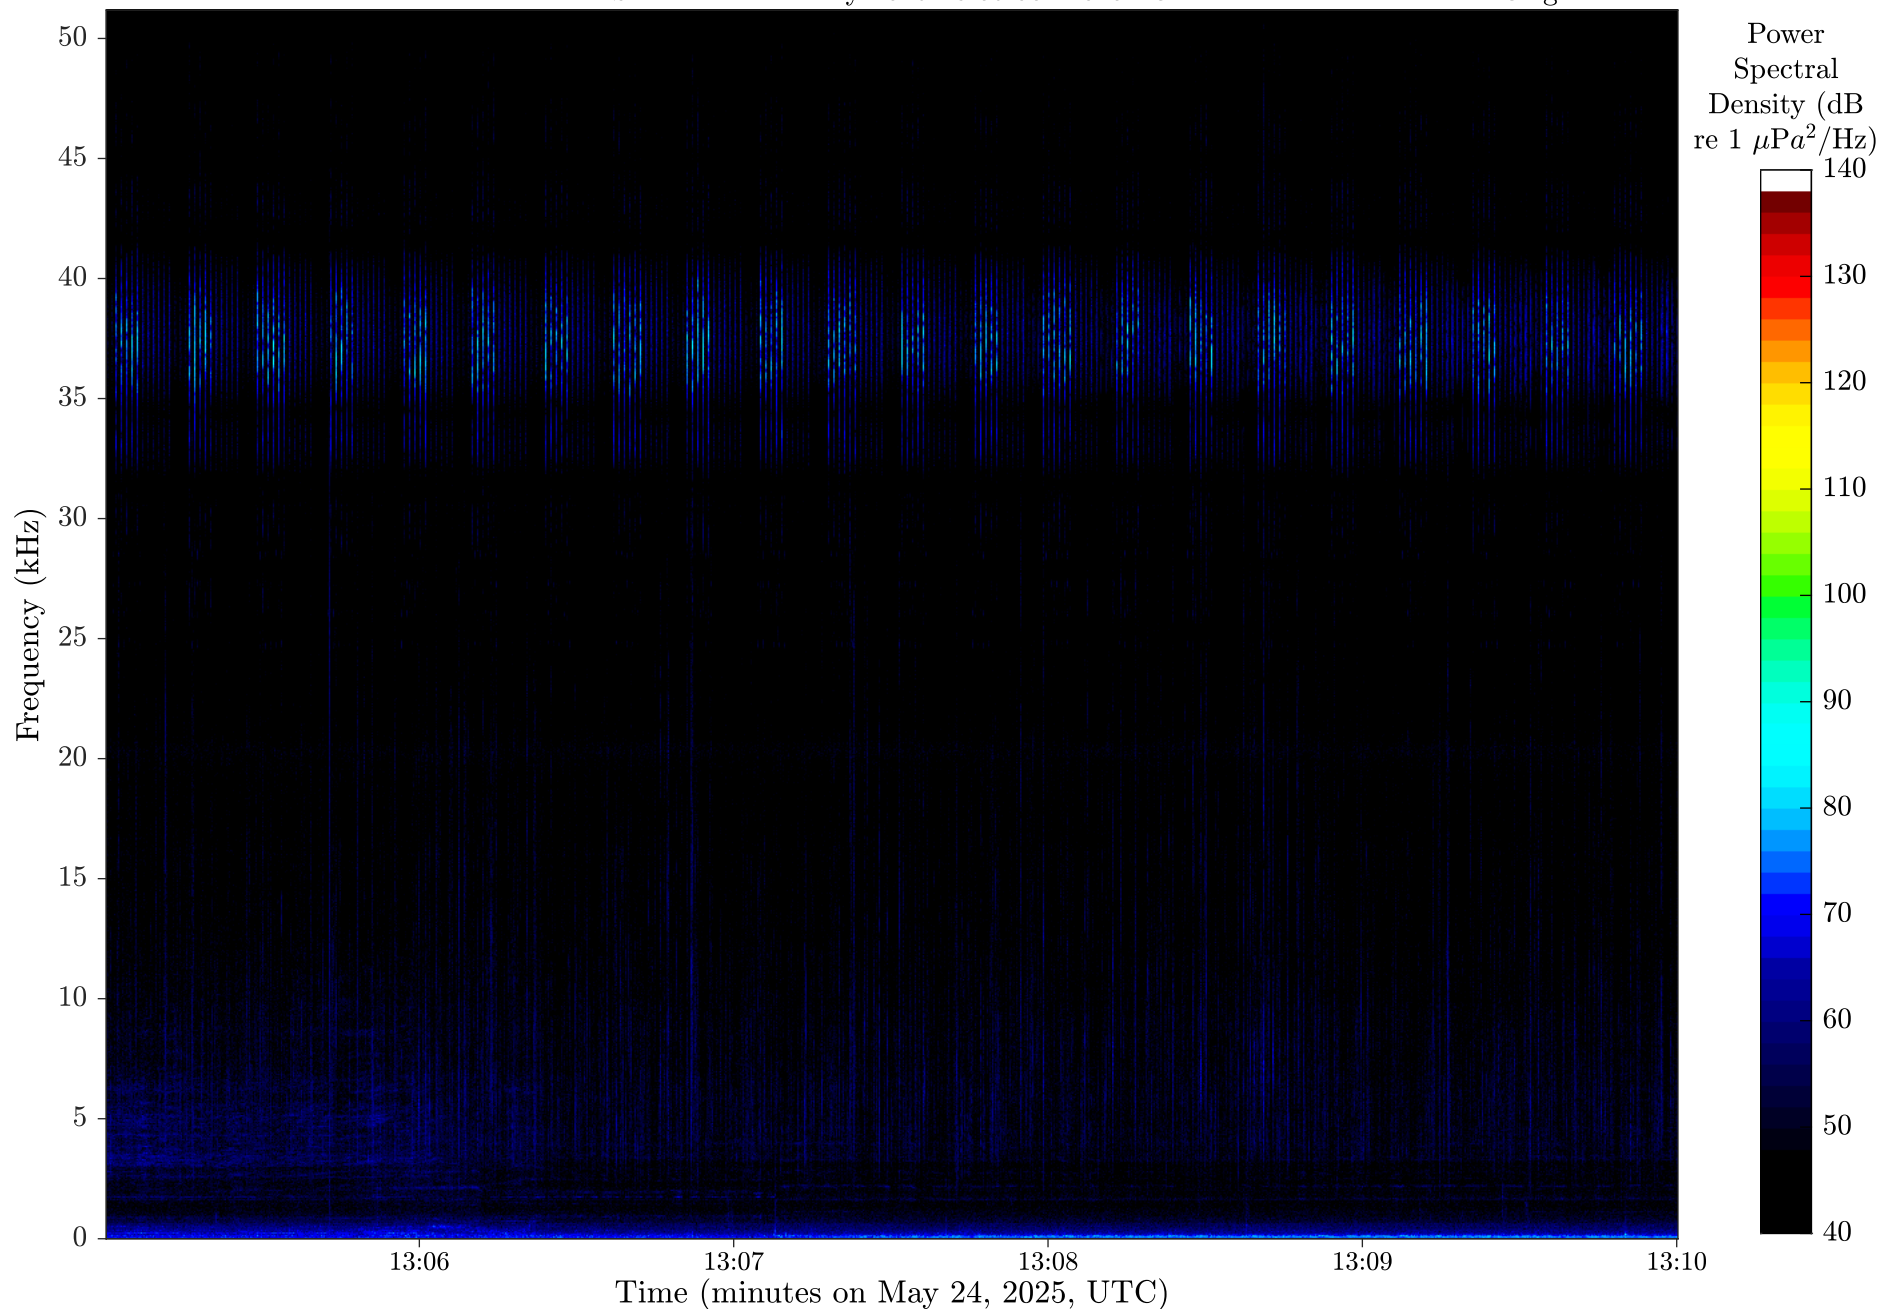

Comments: 31.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:28:49 UTC

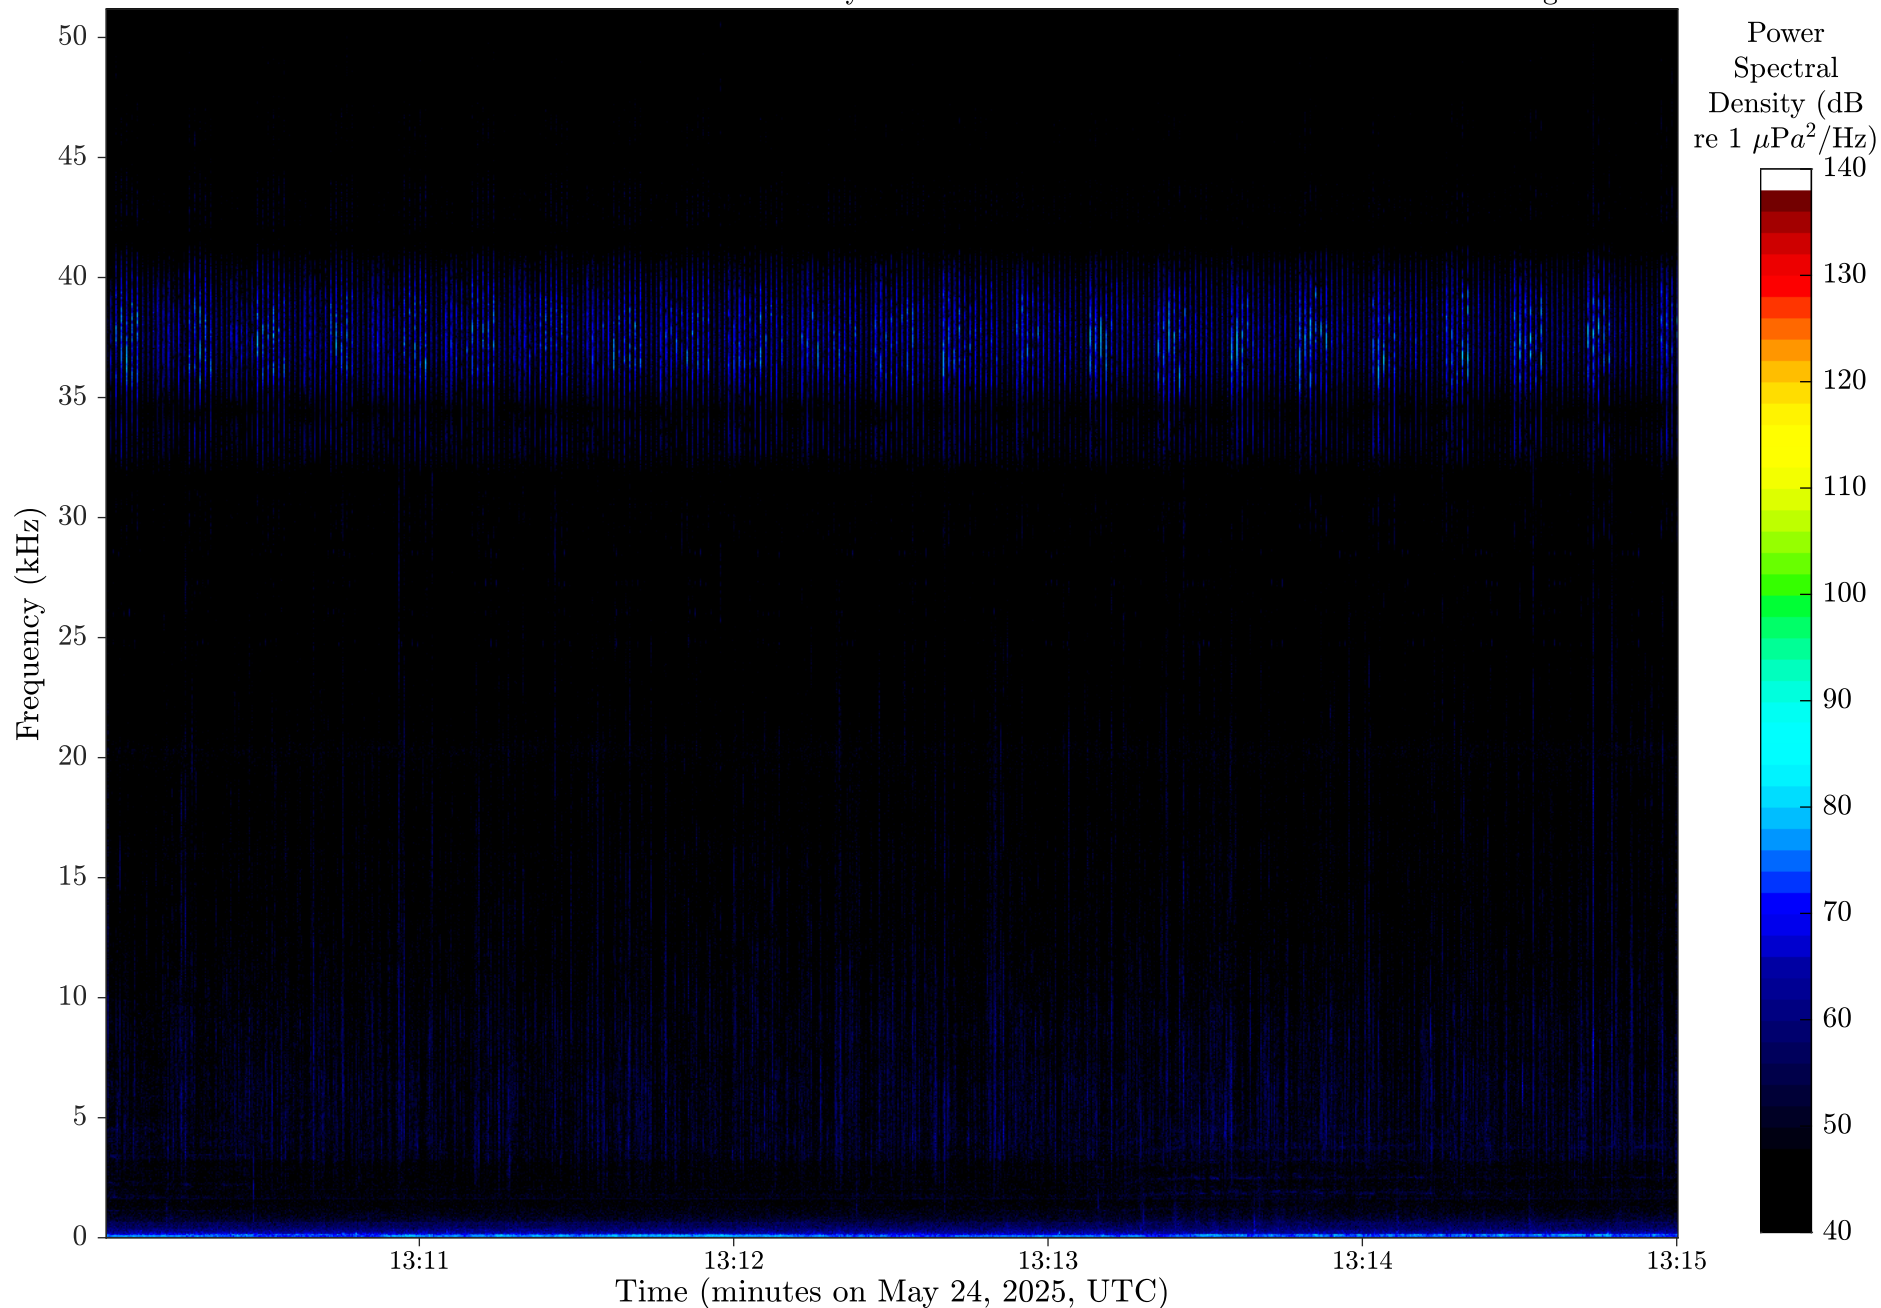

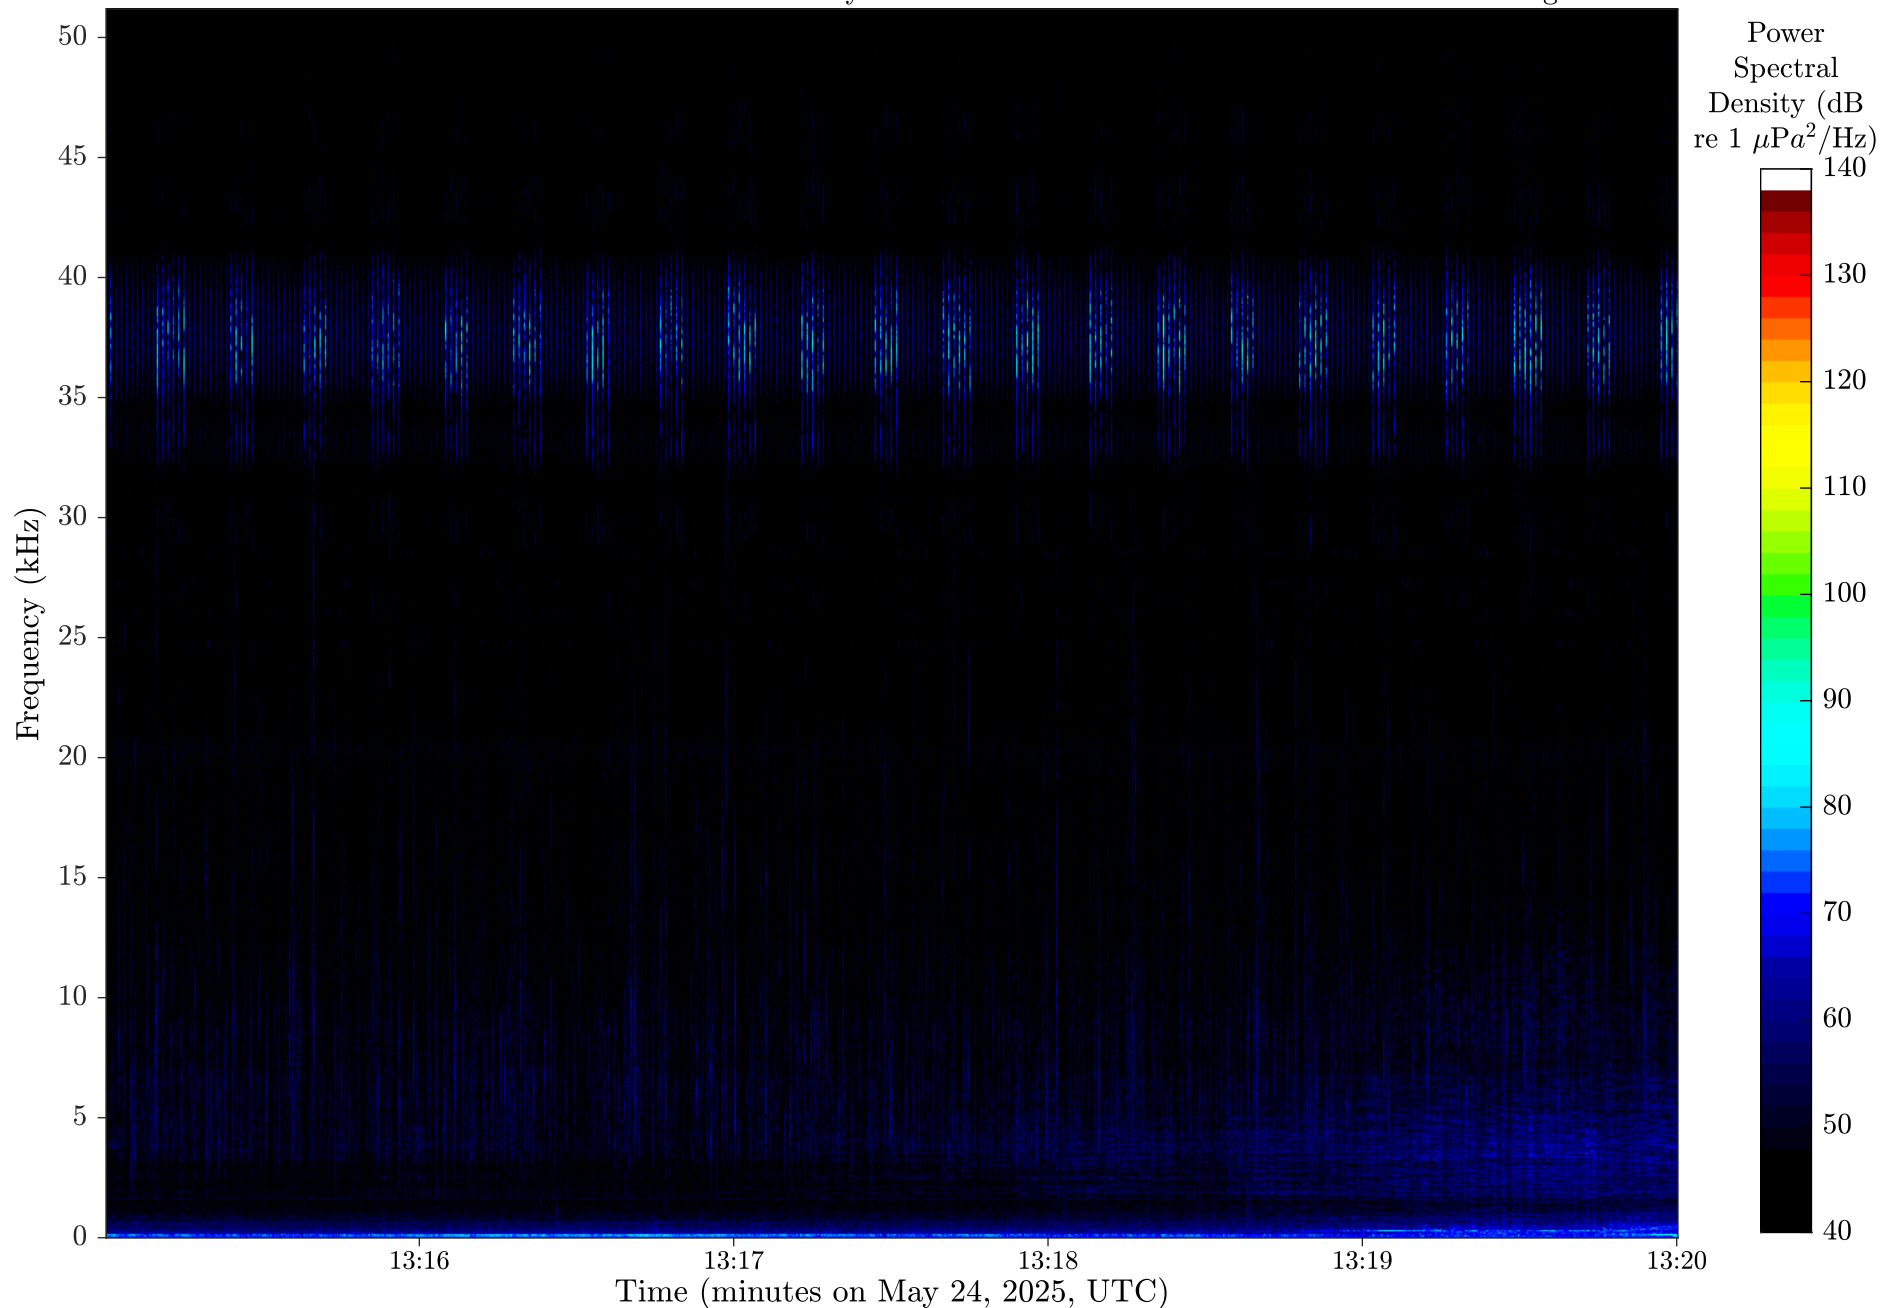


Comments: 30.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:06 UTC

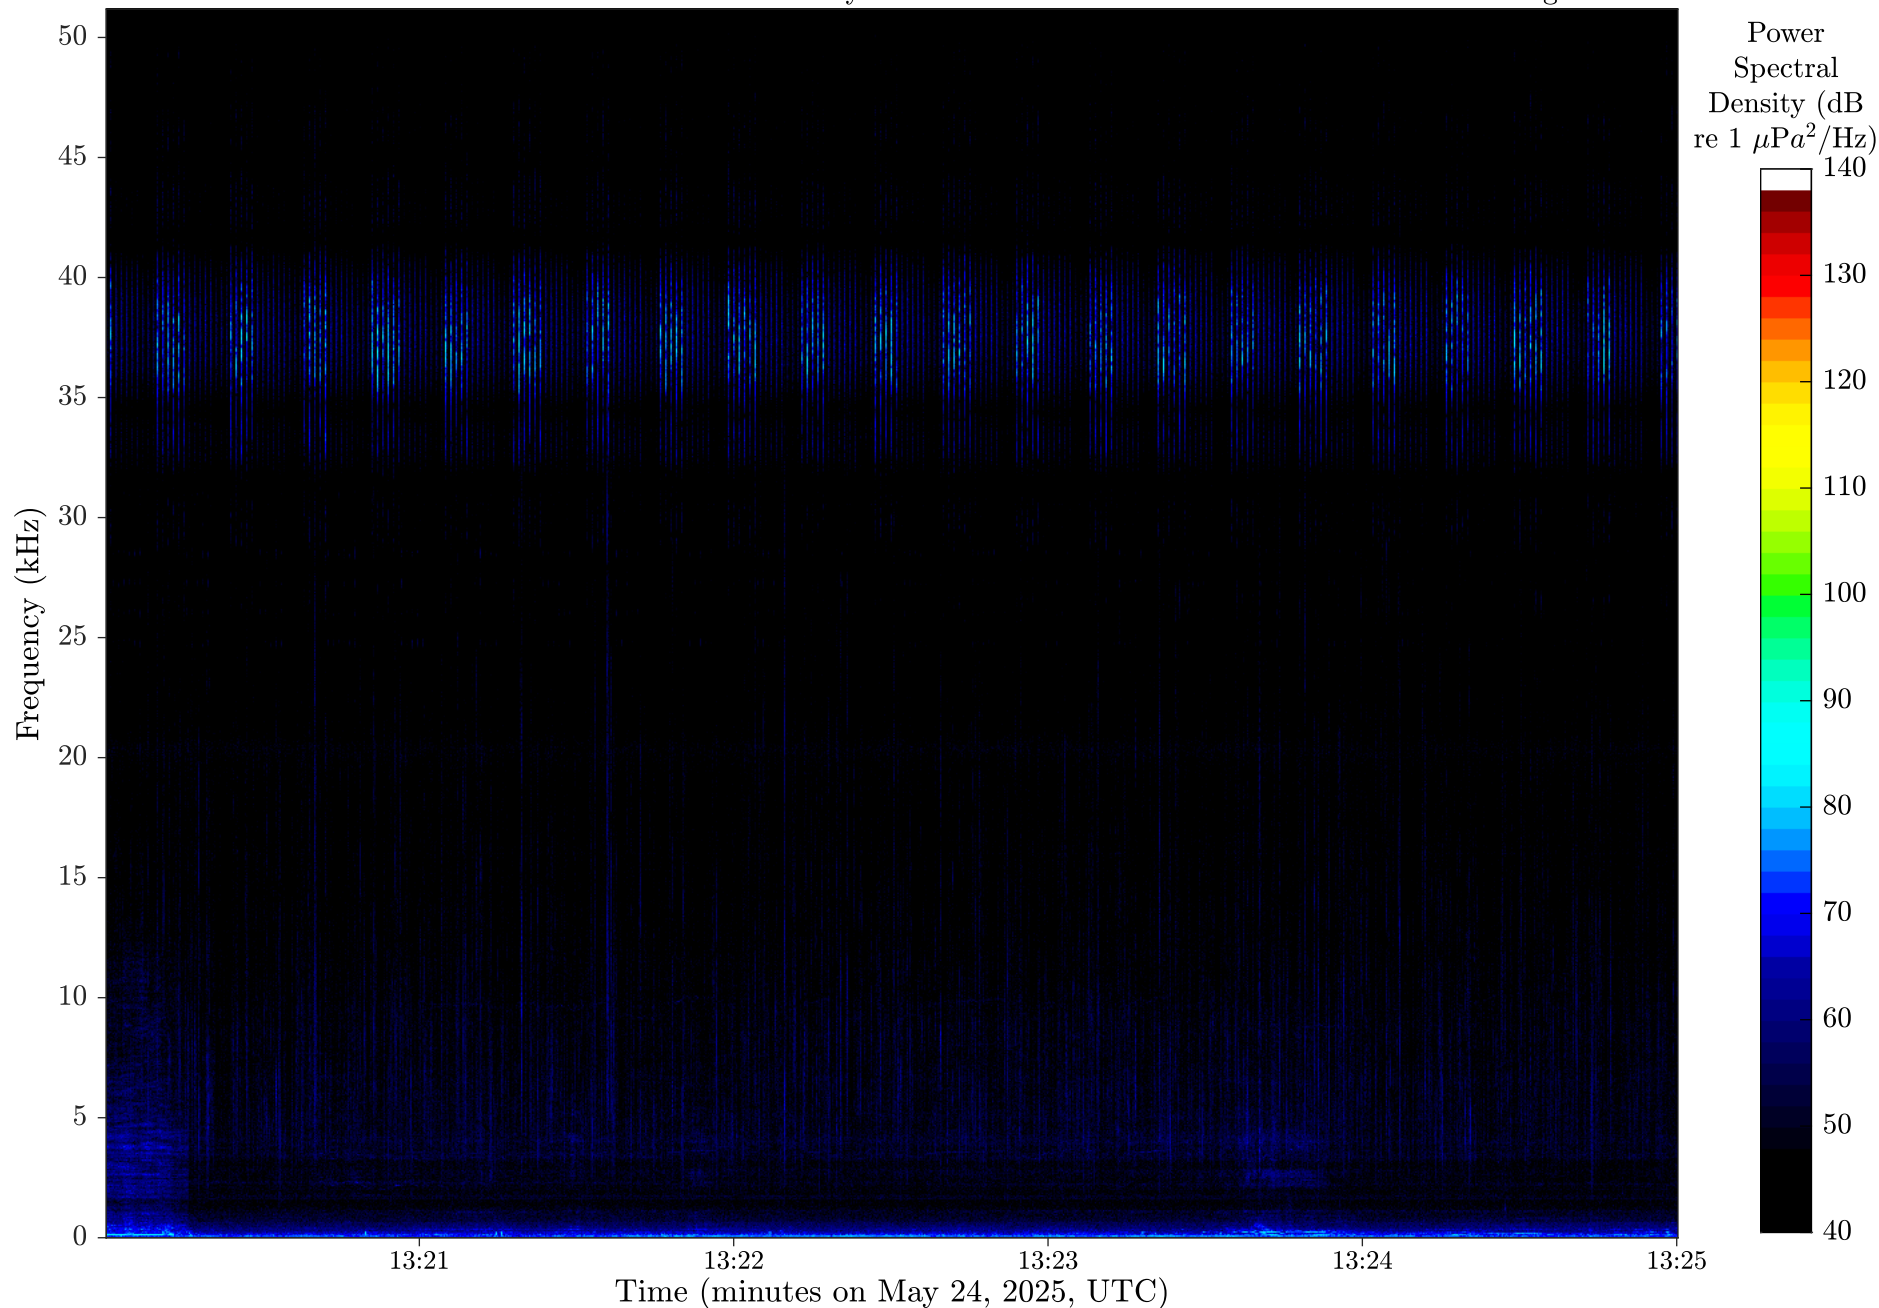


Comments: 31.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:29:13 UTC

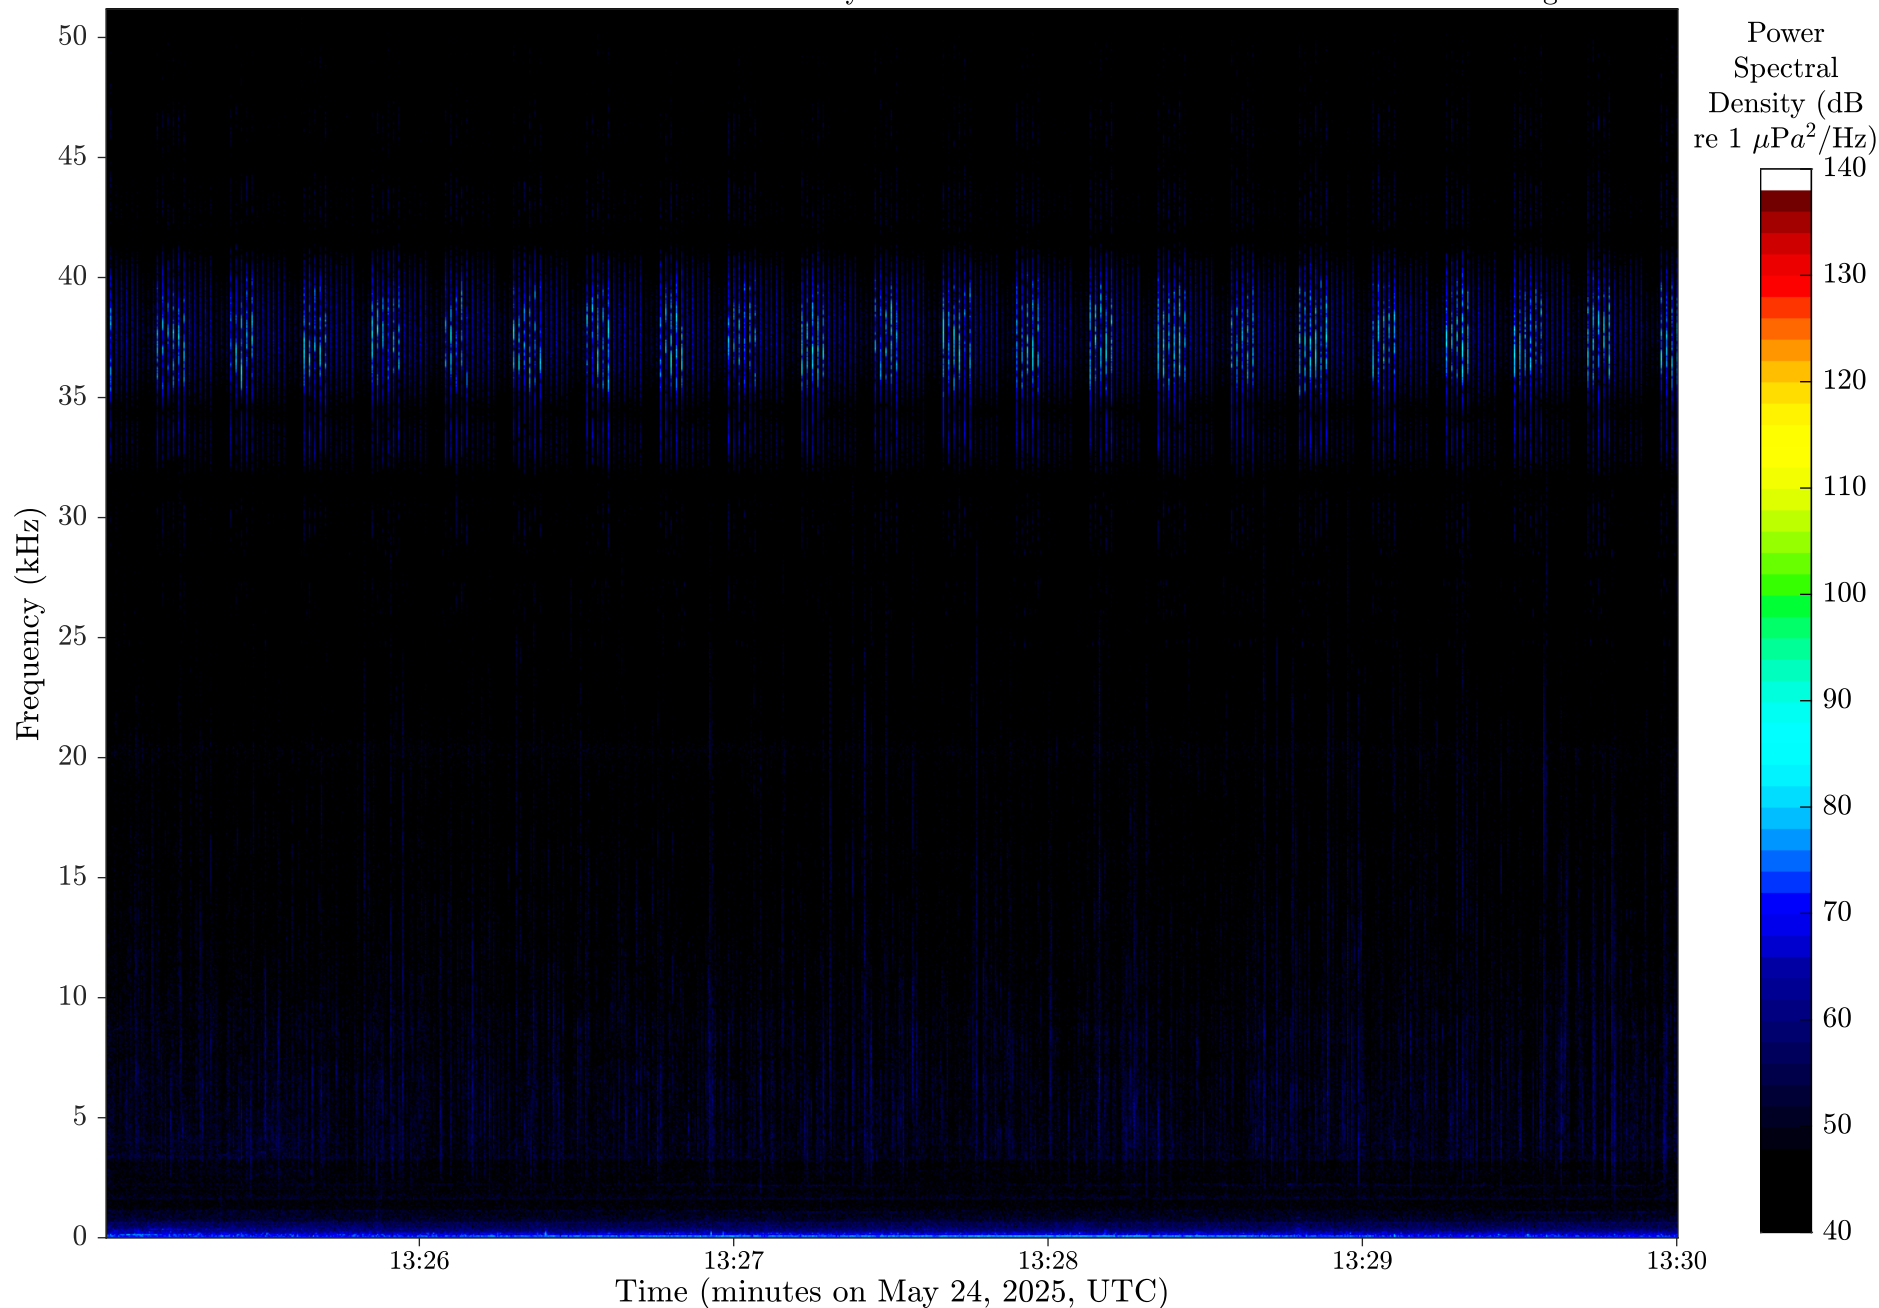

Comments: 32.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:29:20 UTC

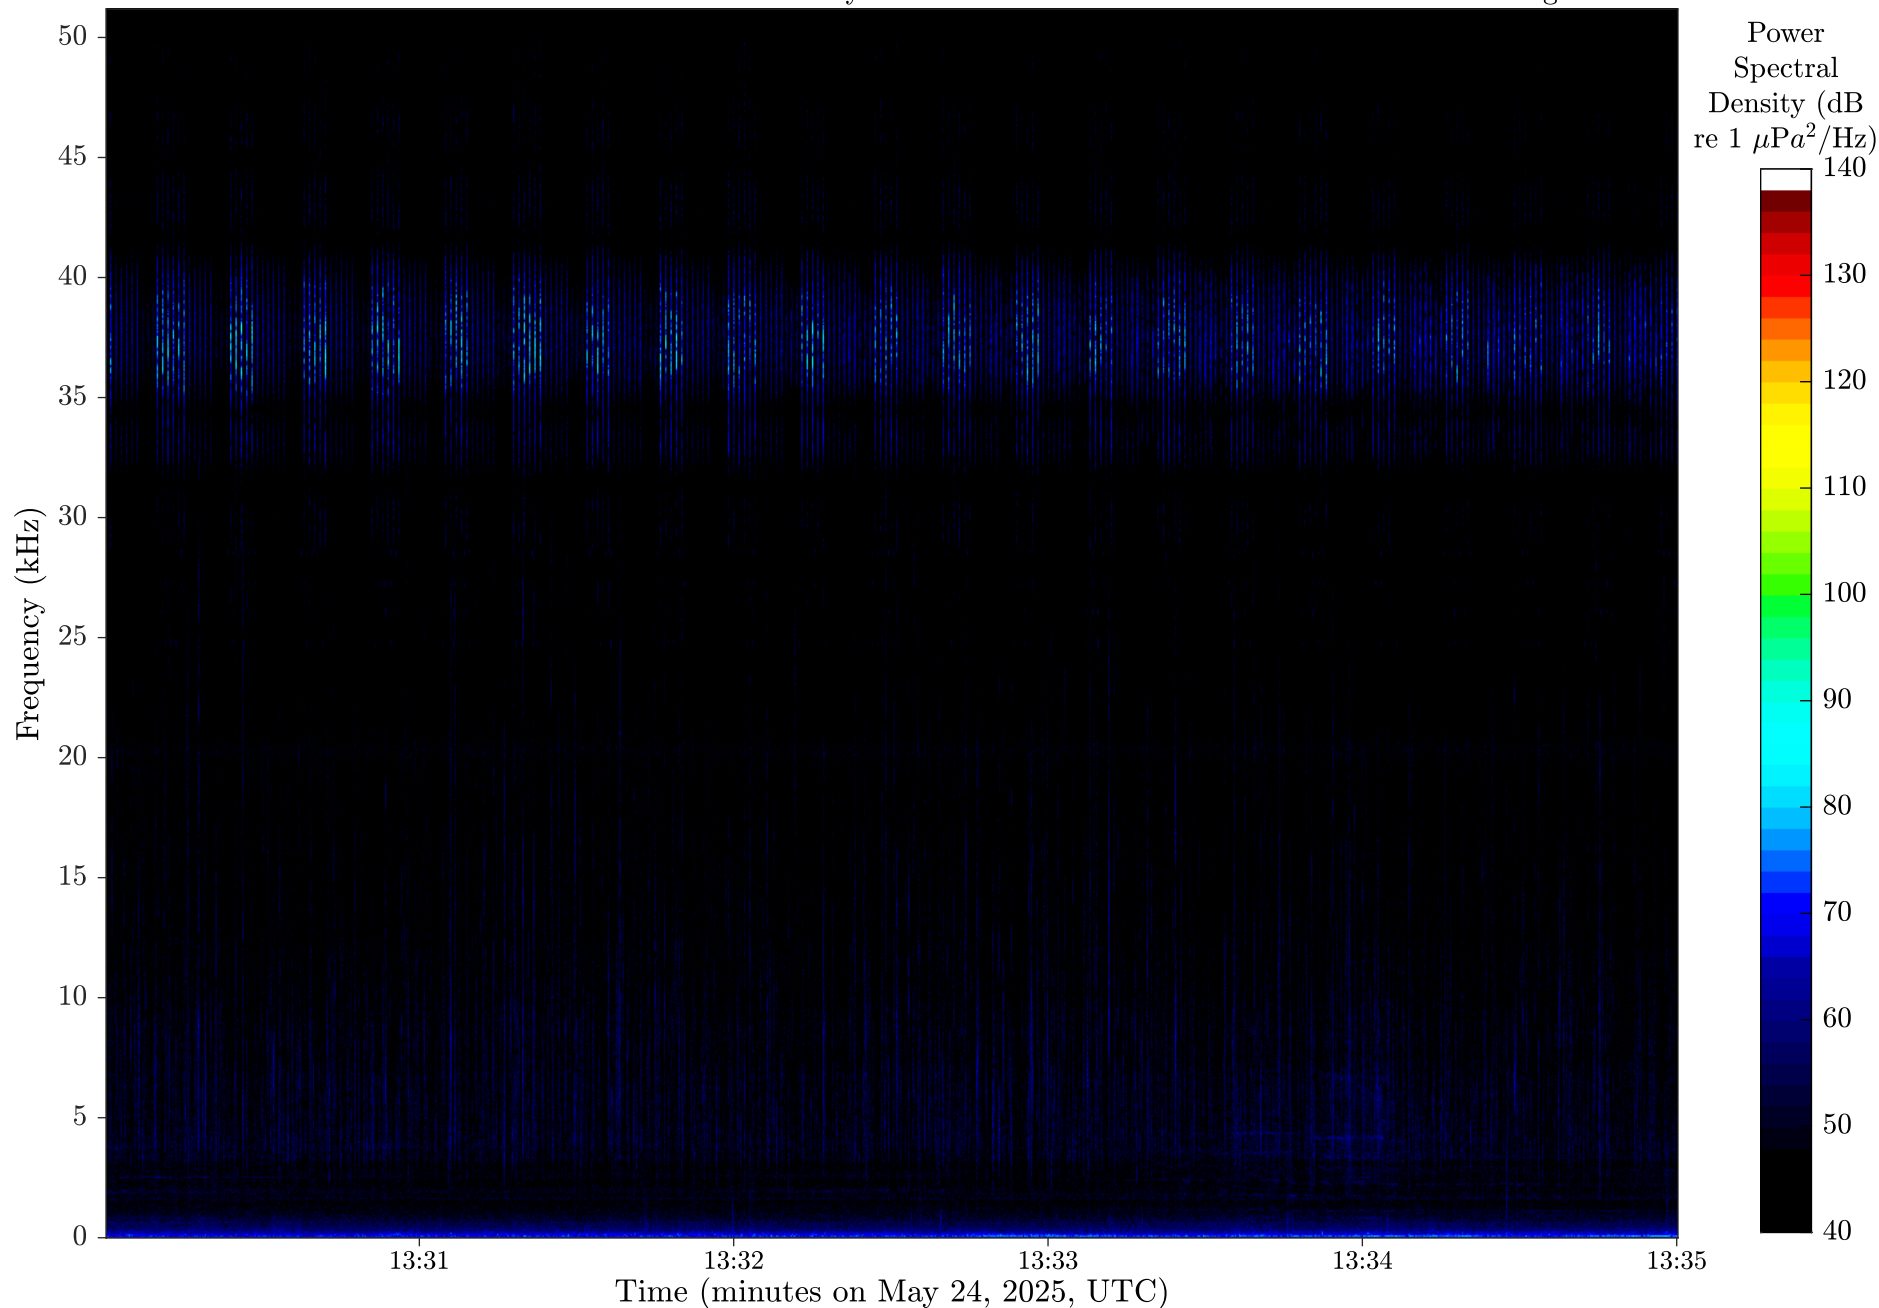

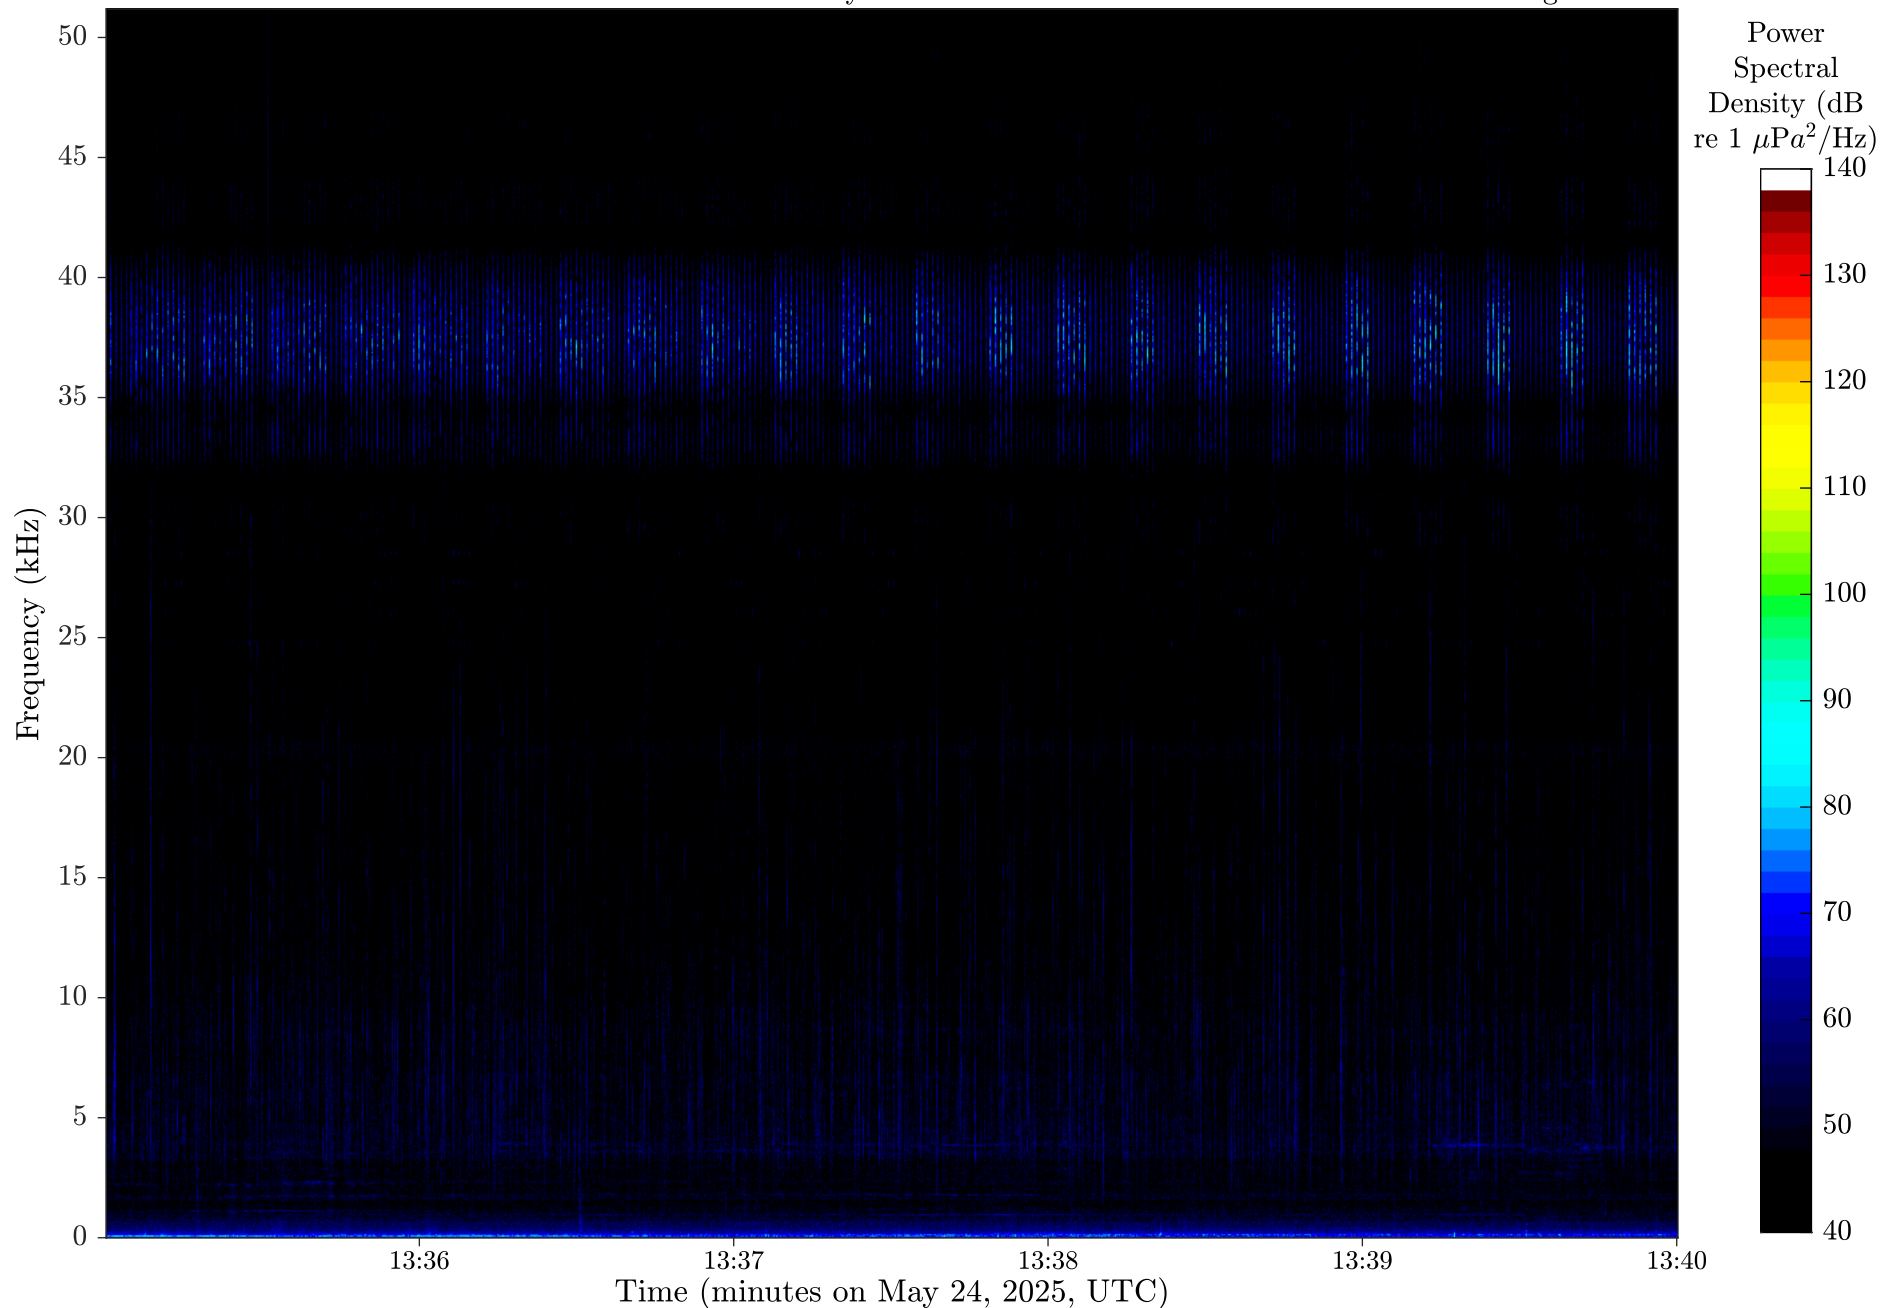


Comments: 30.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:36 UTC

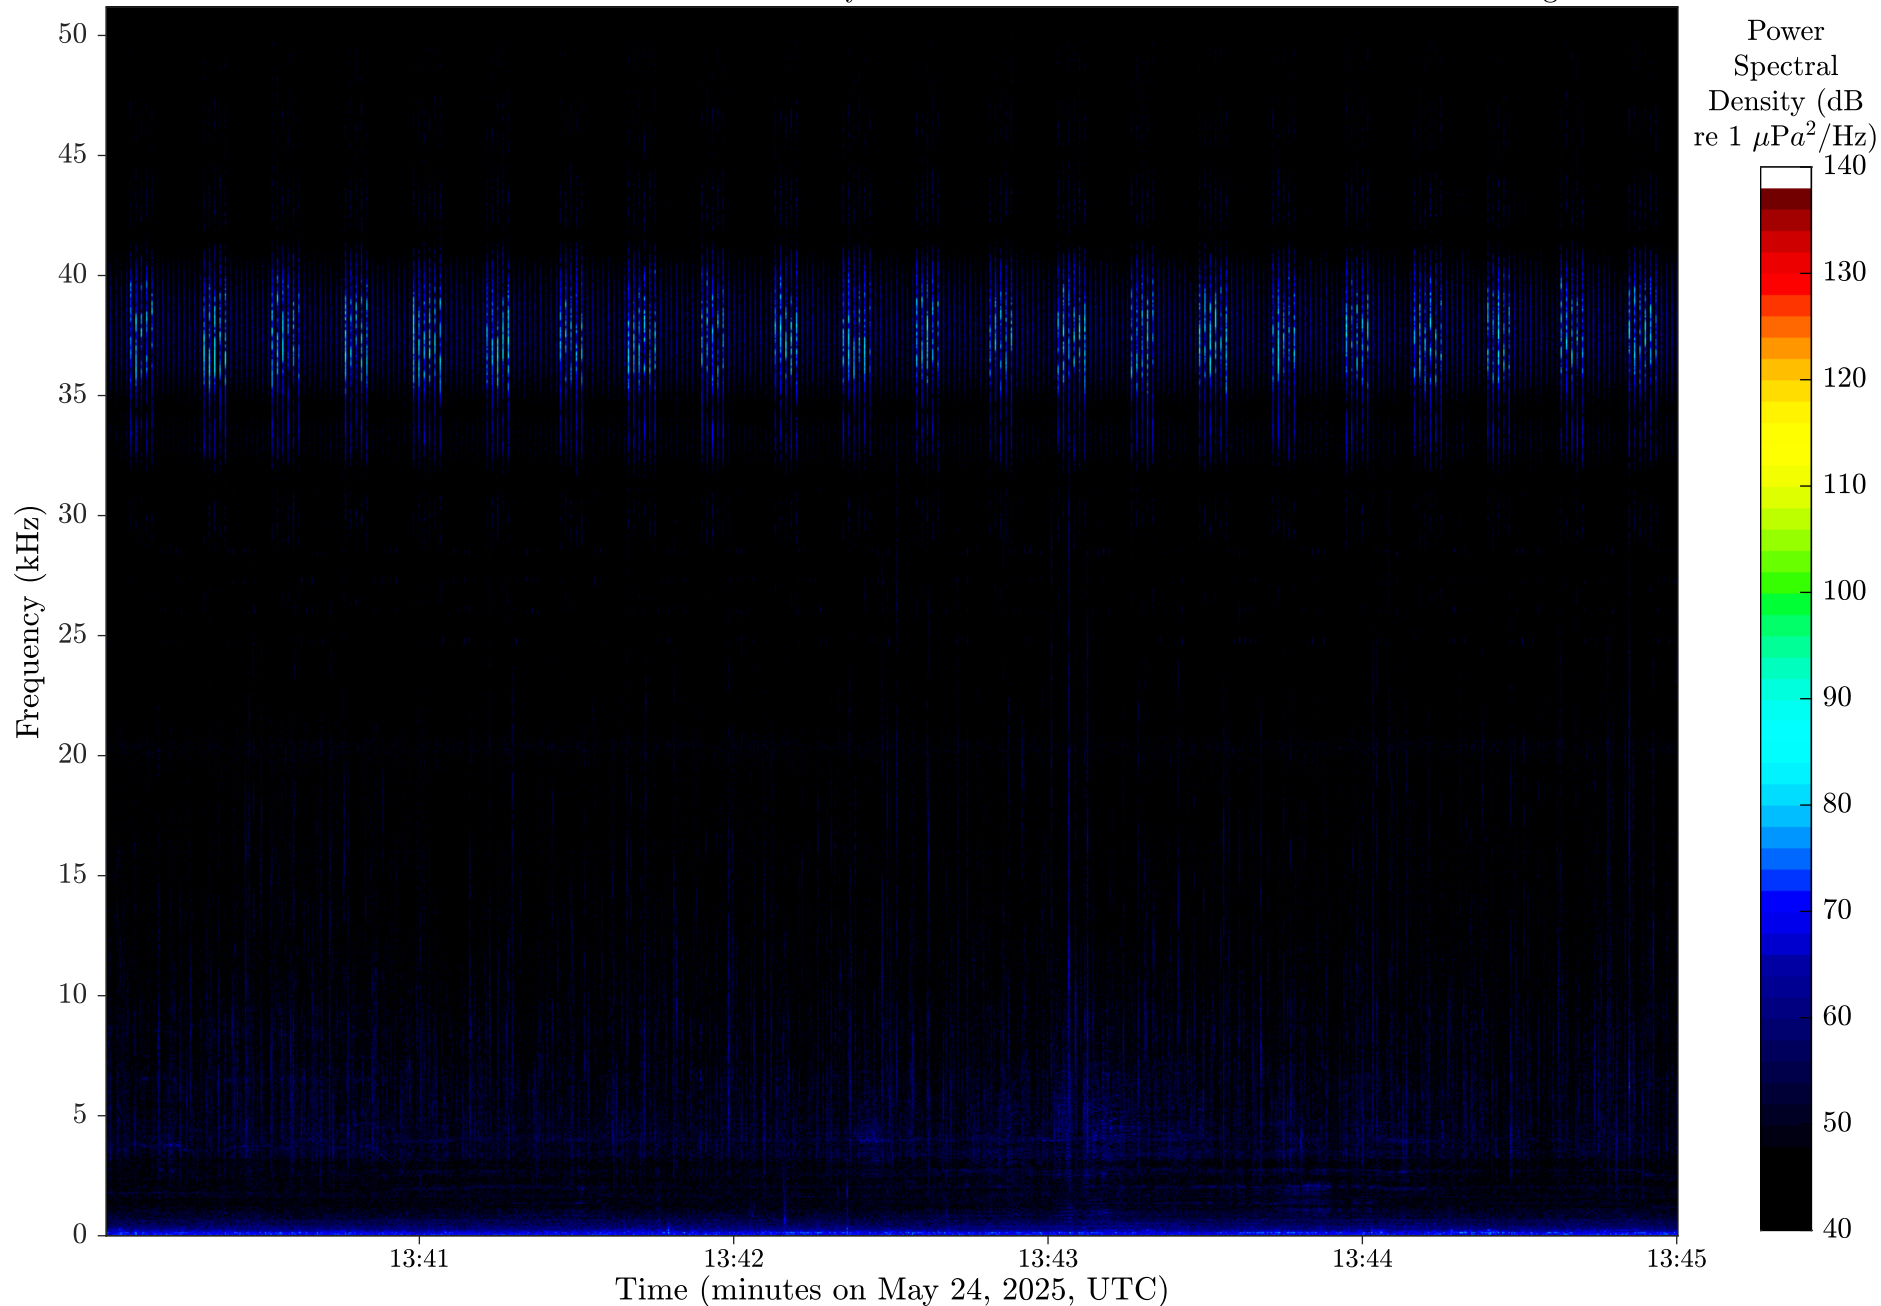


Comments: 31.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:45 UTC

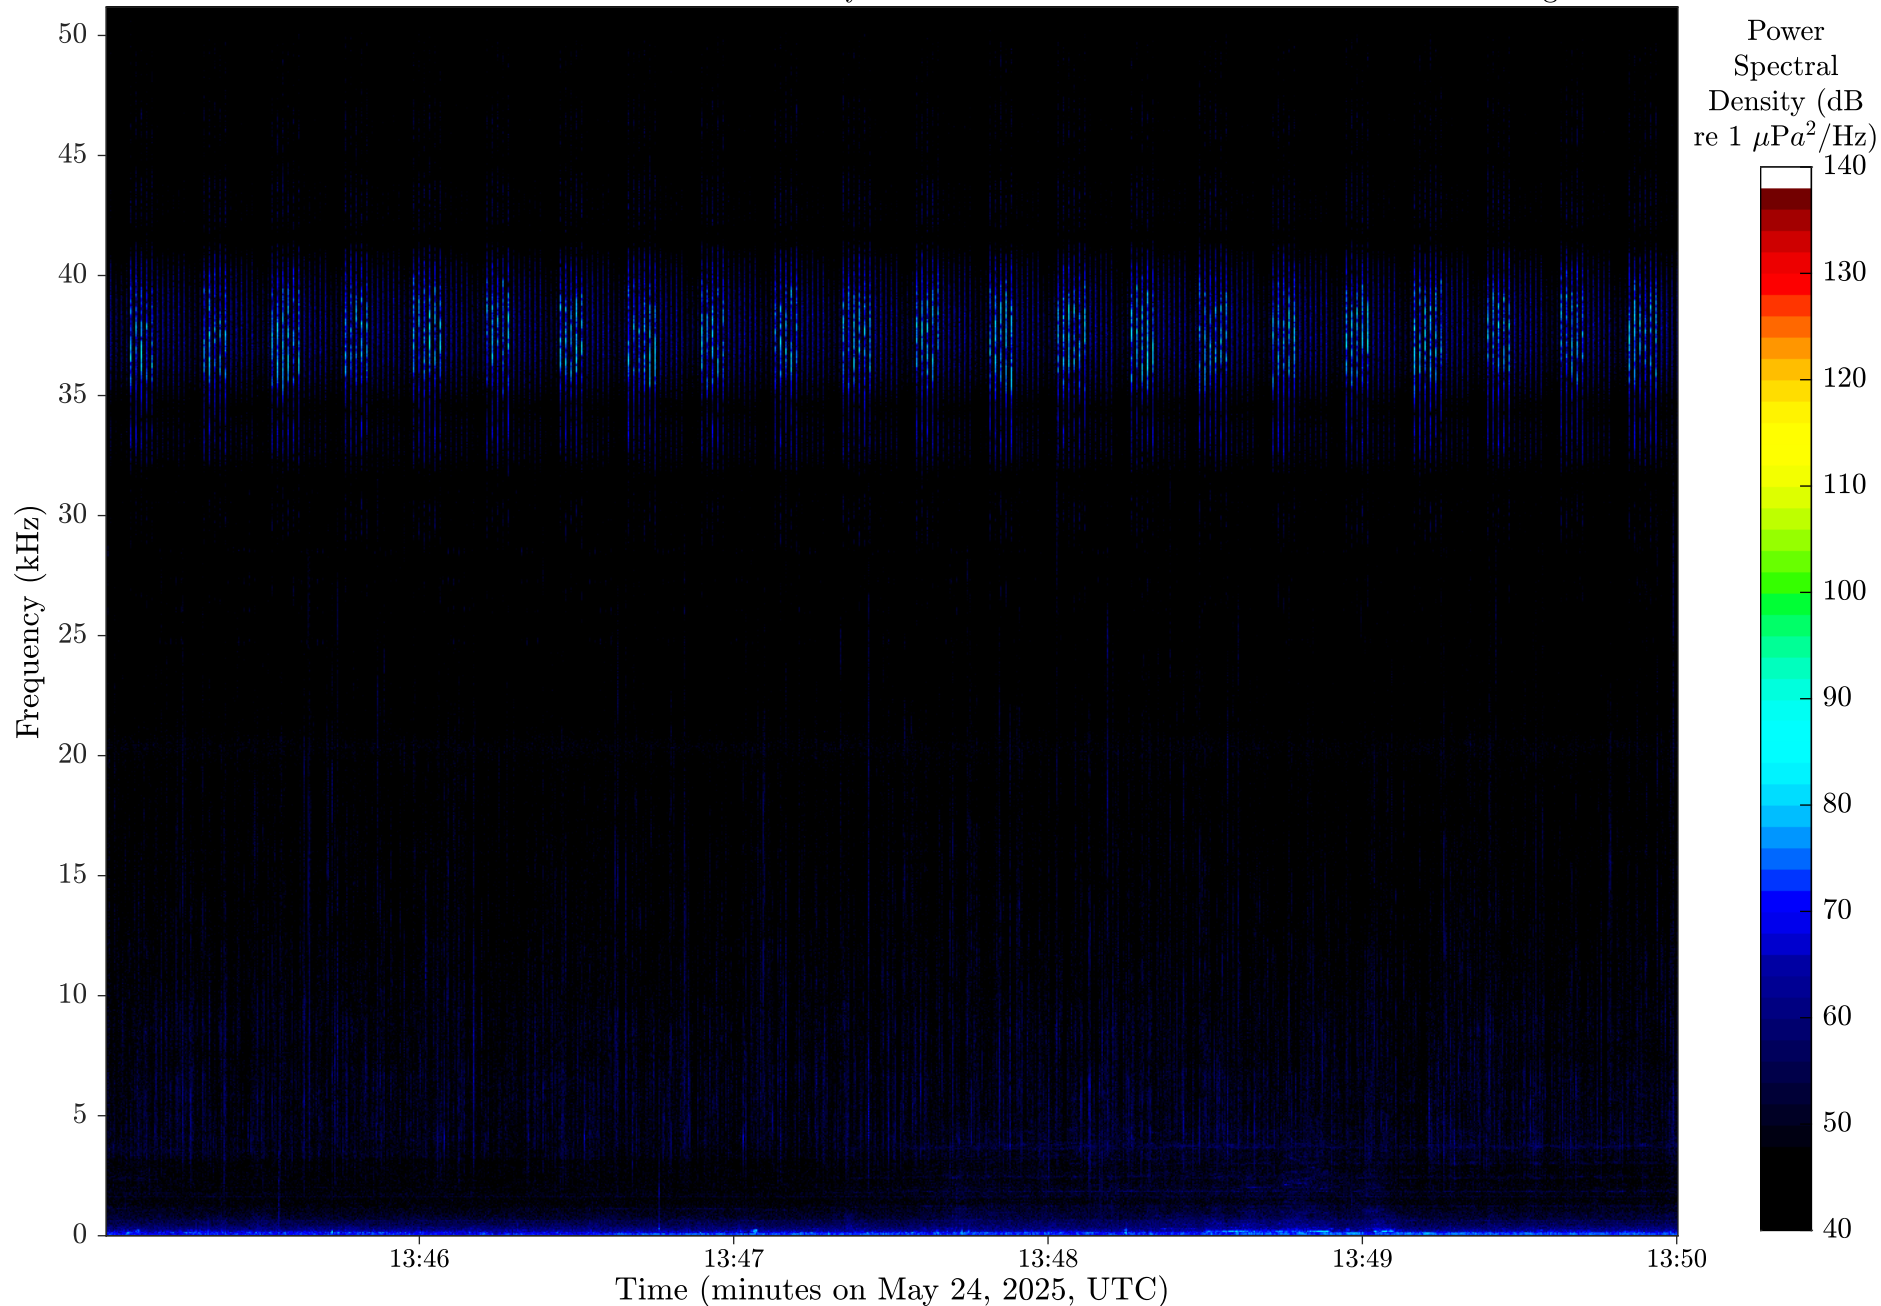


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:52 UTC

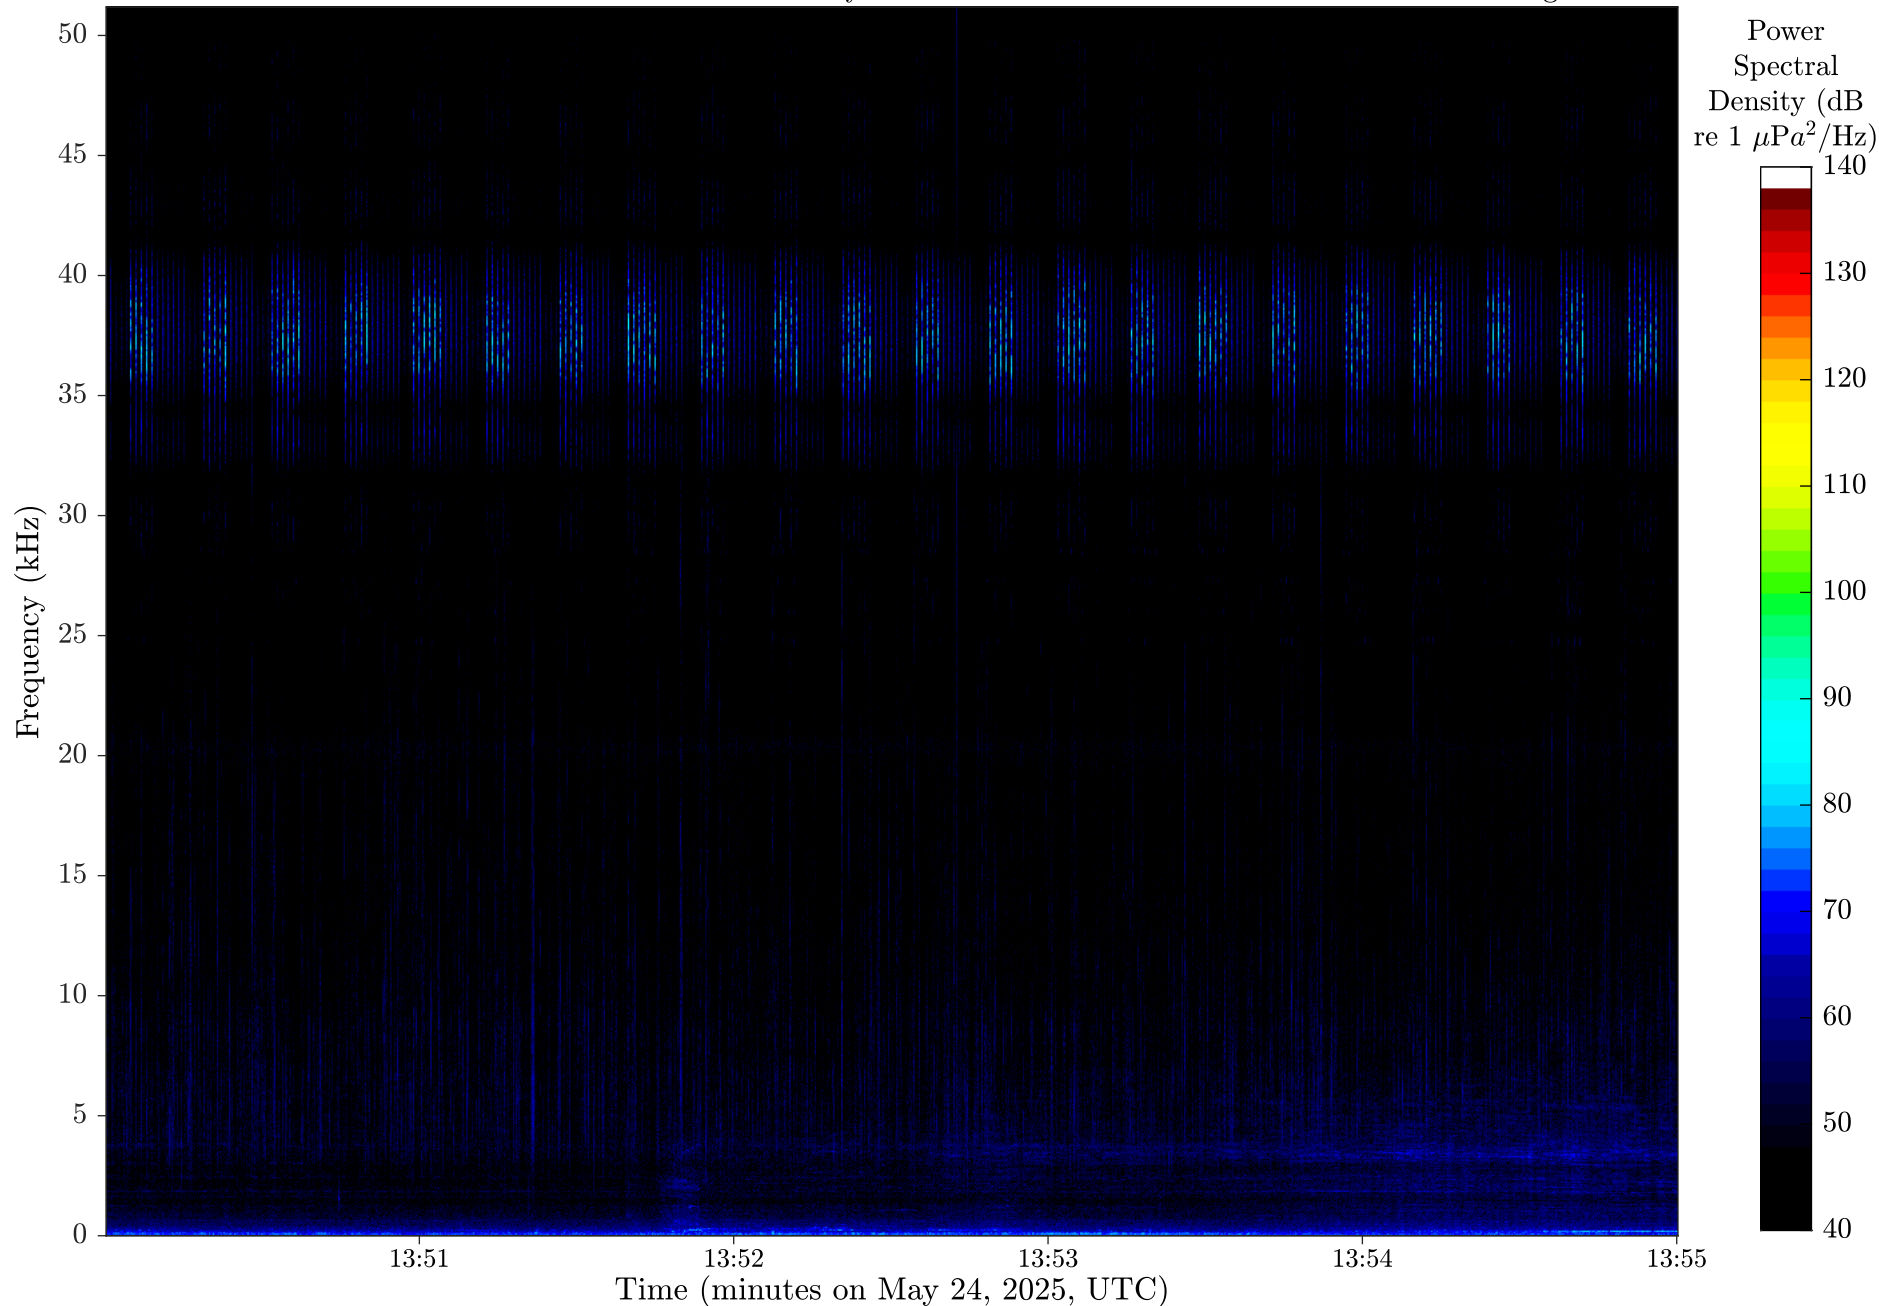


Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:30:01 UTC

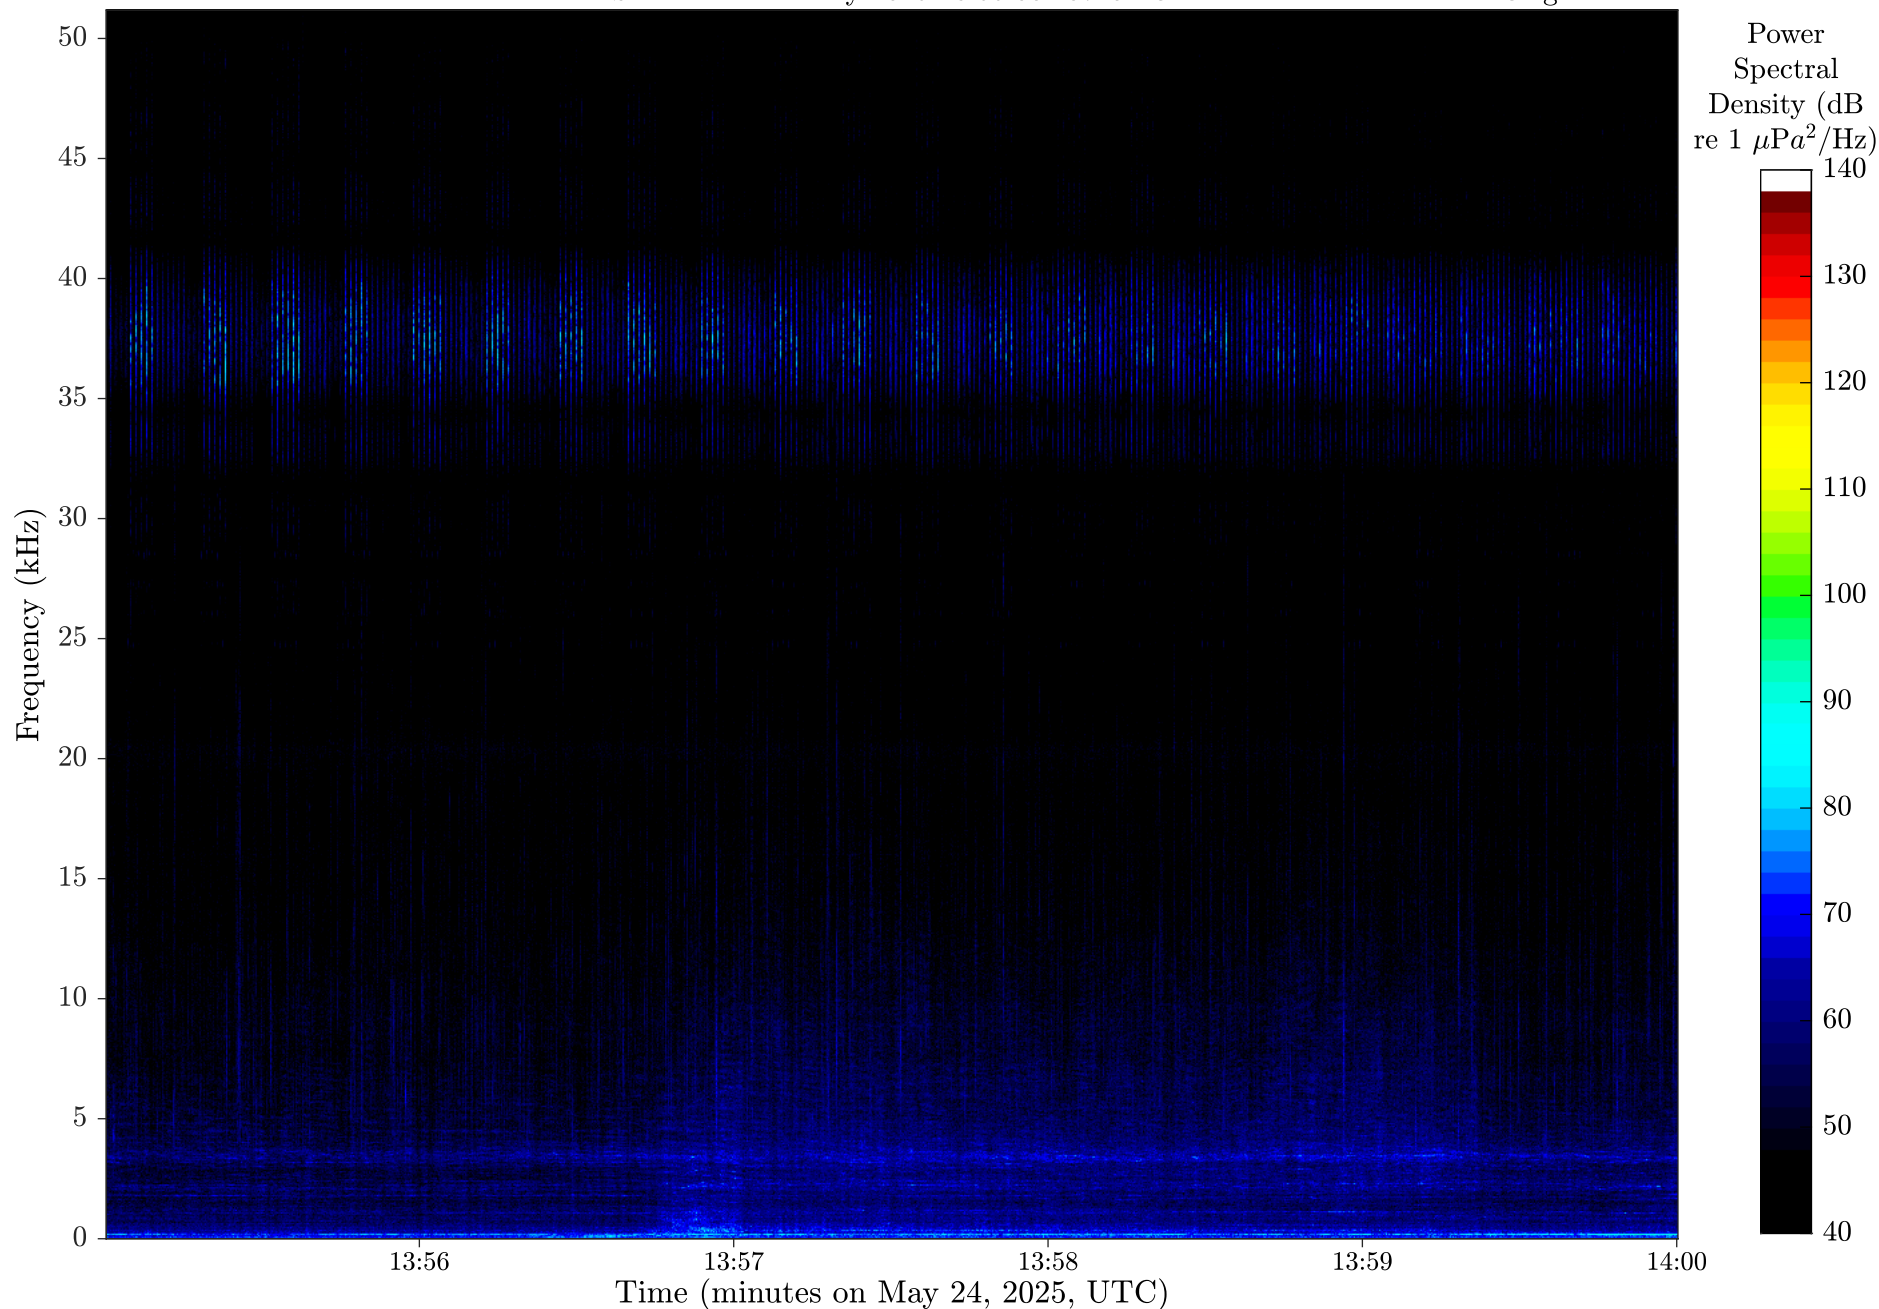


Comments: 29.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:30:10 UTC

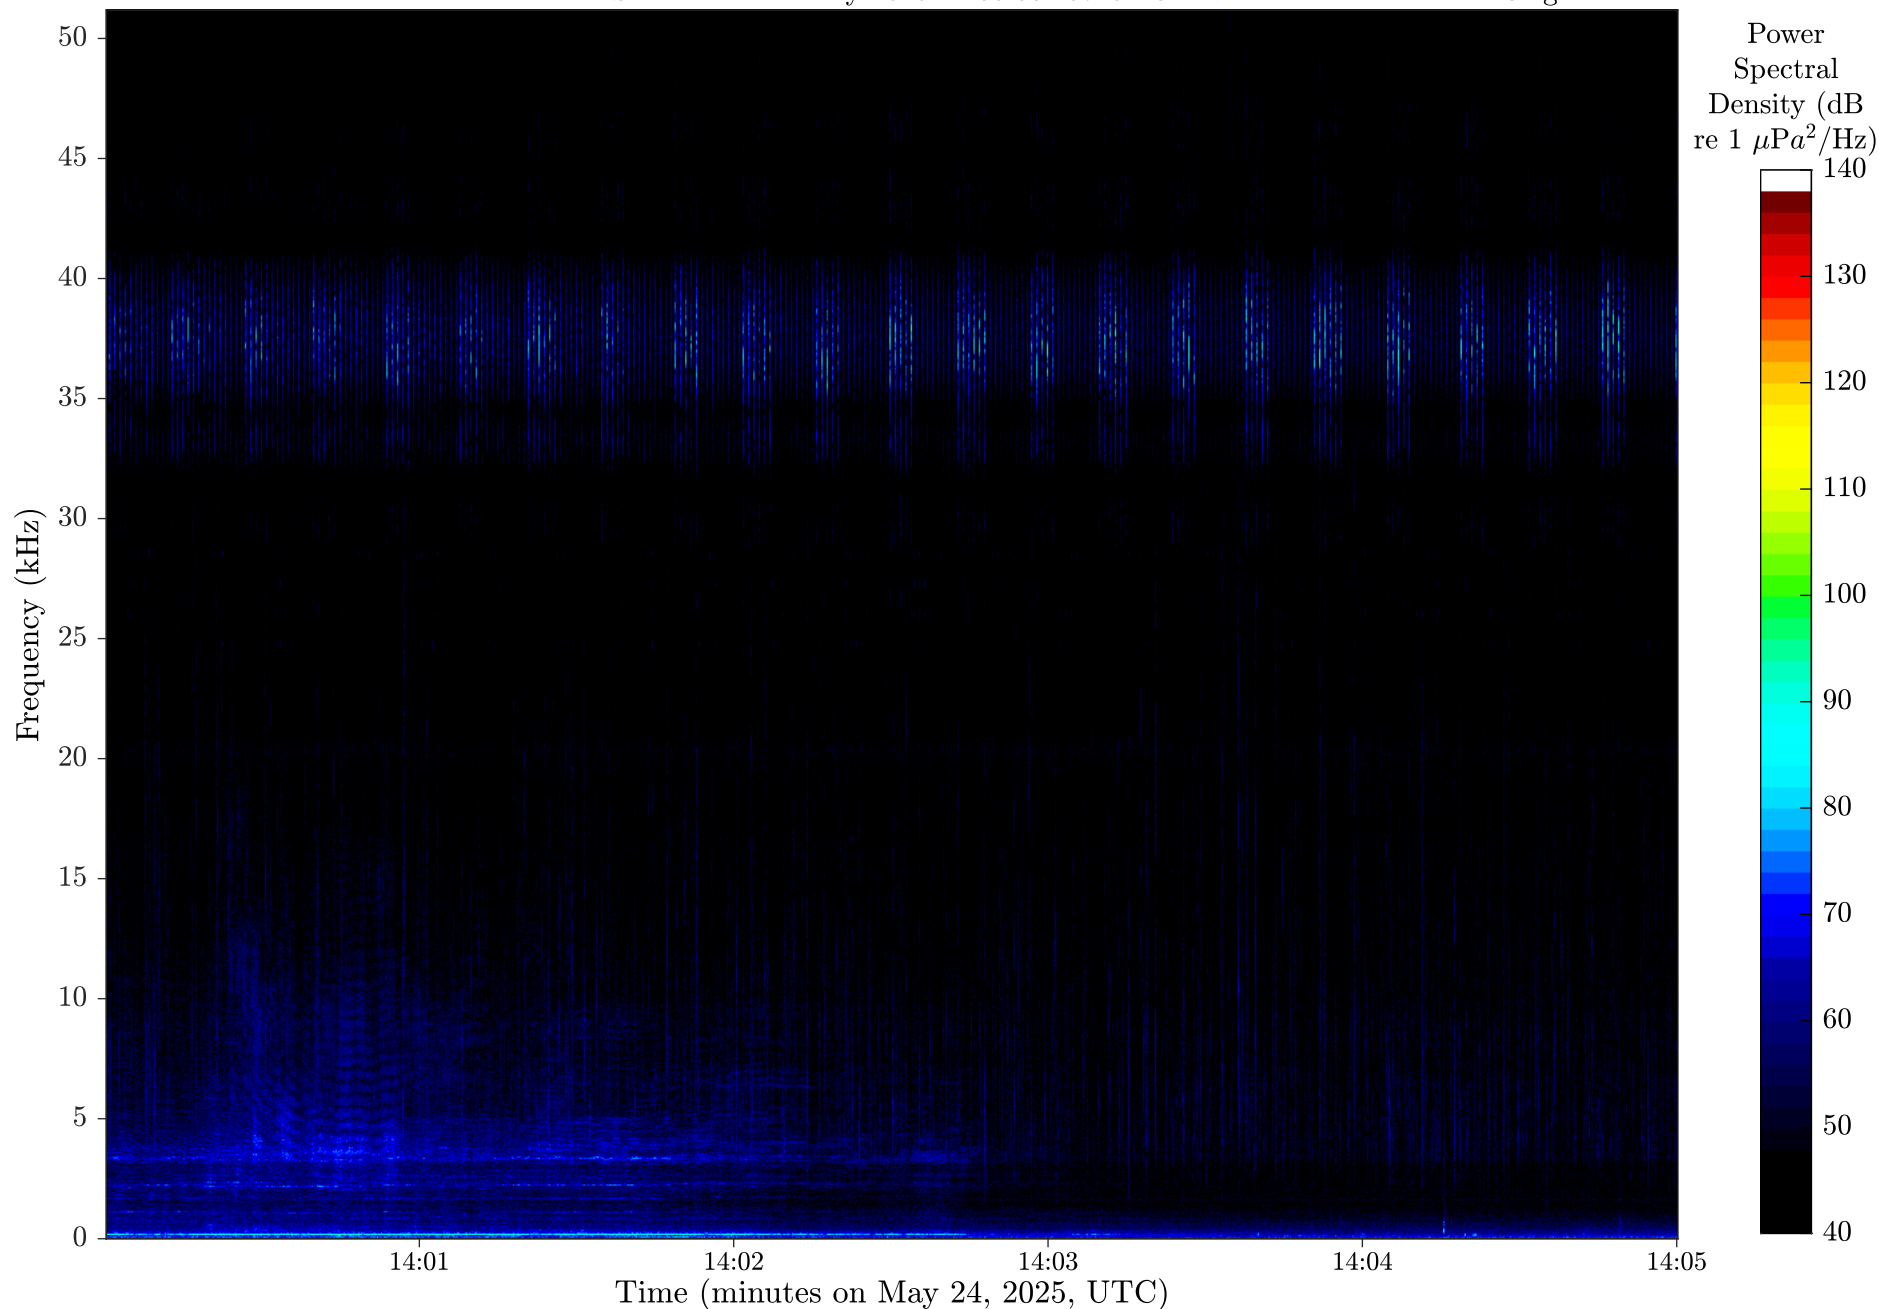


Comments: 31.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:30:19 UTC

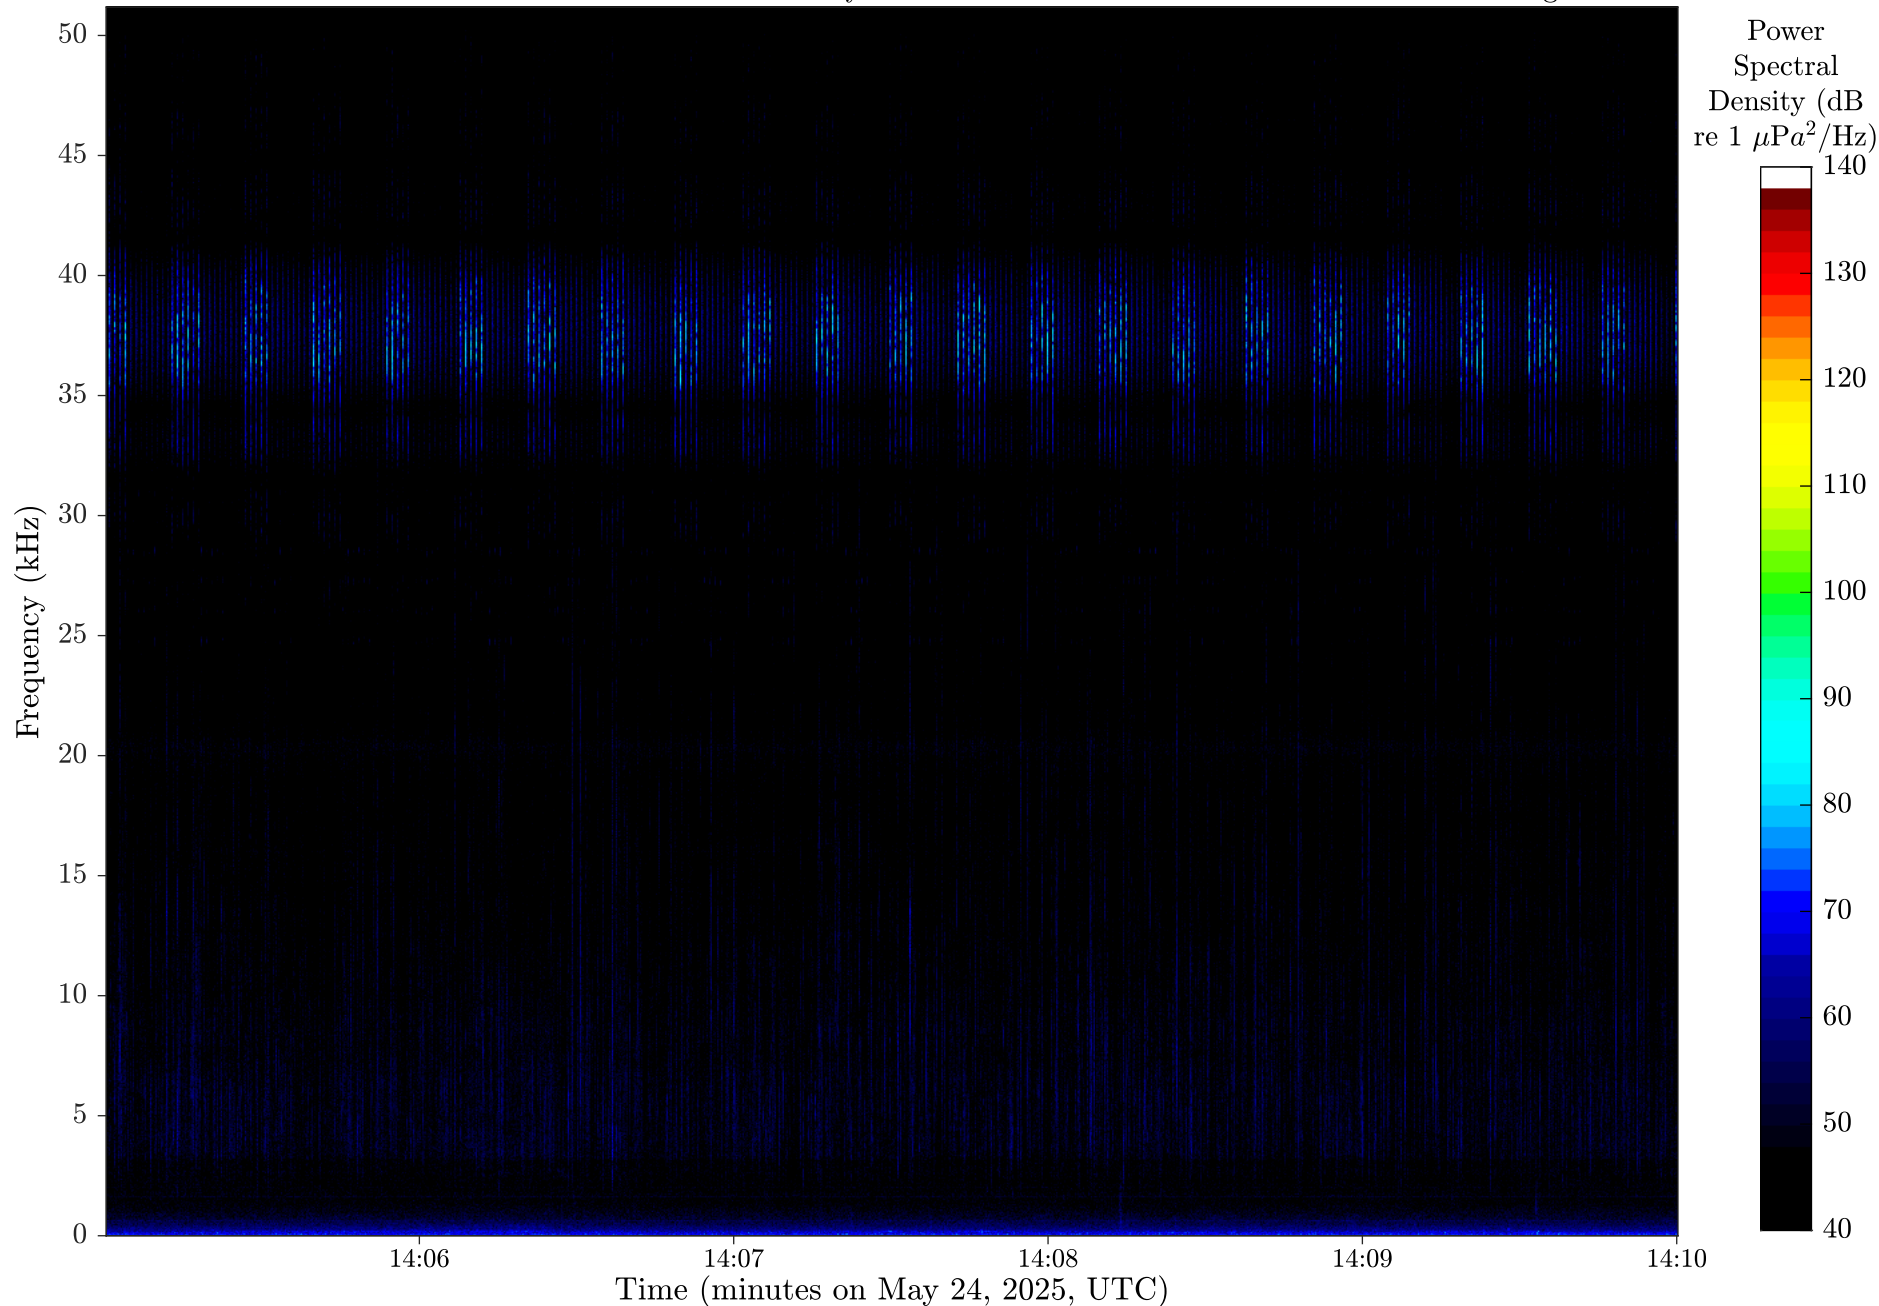


Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:30:26 UTC

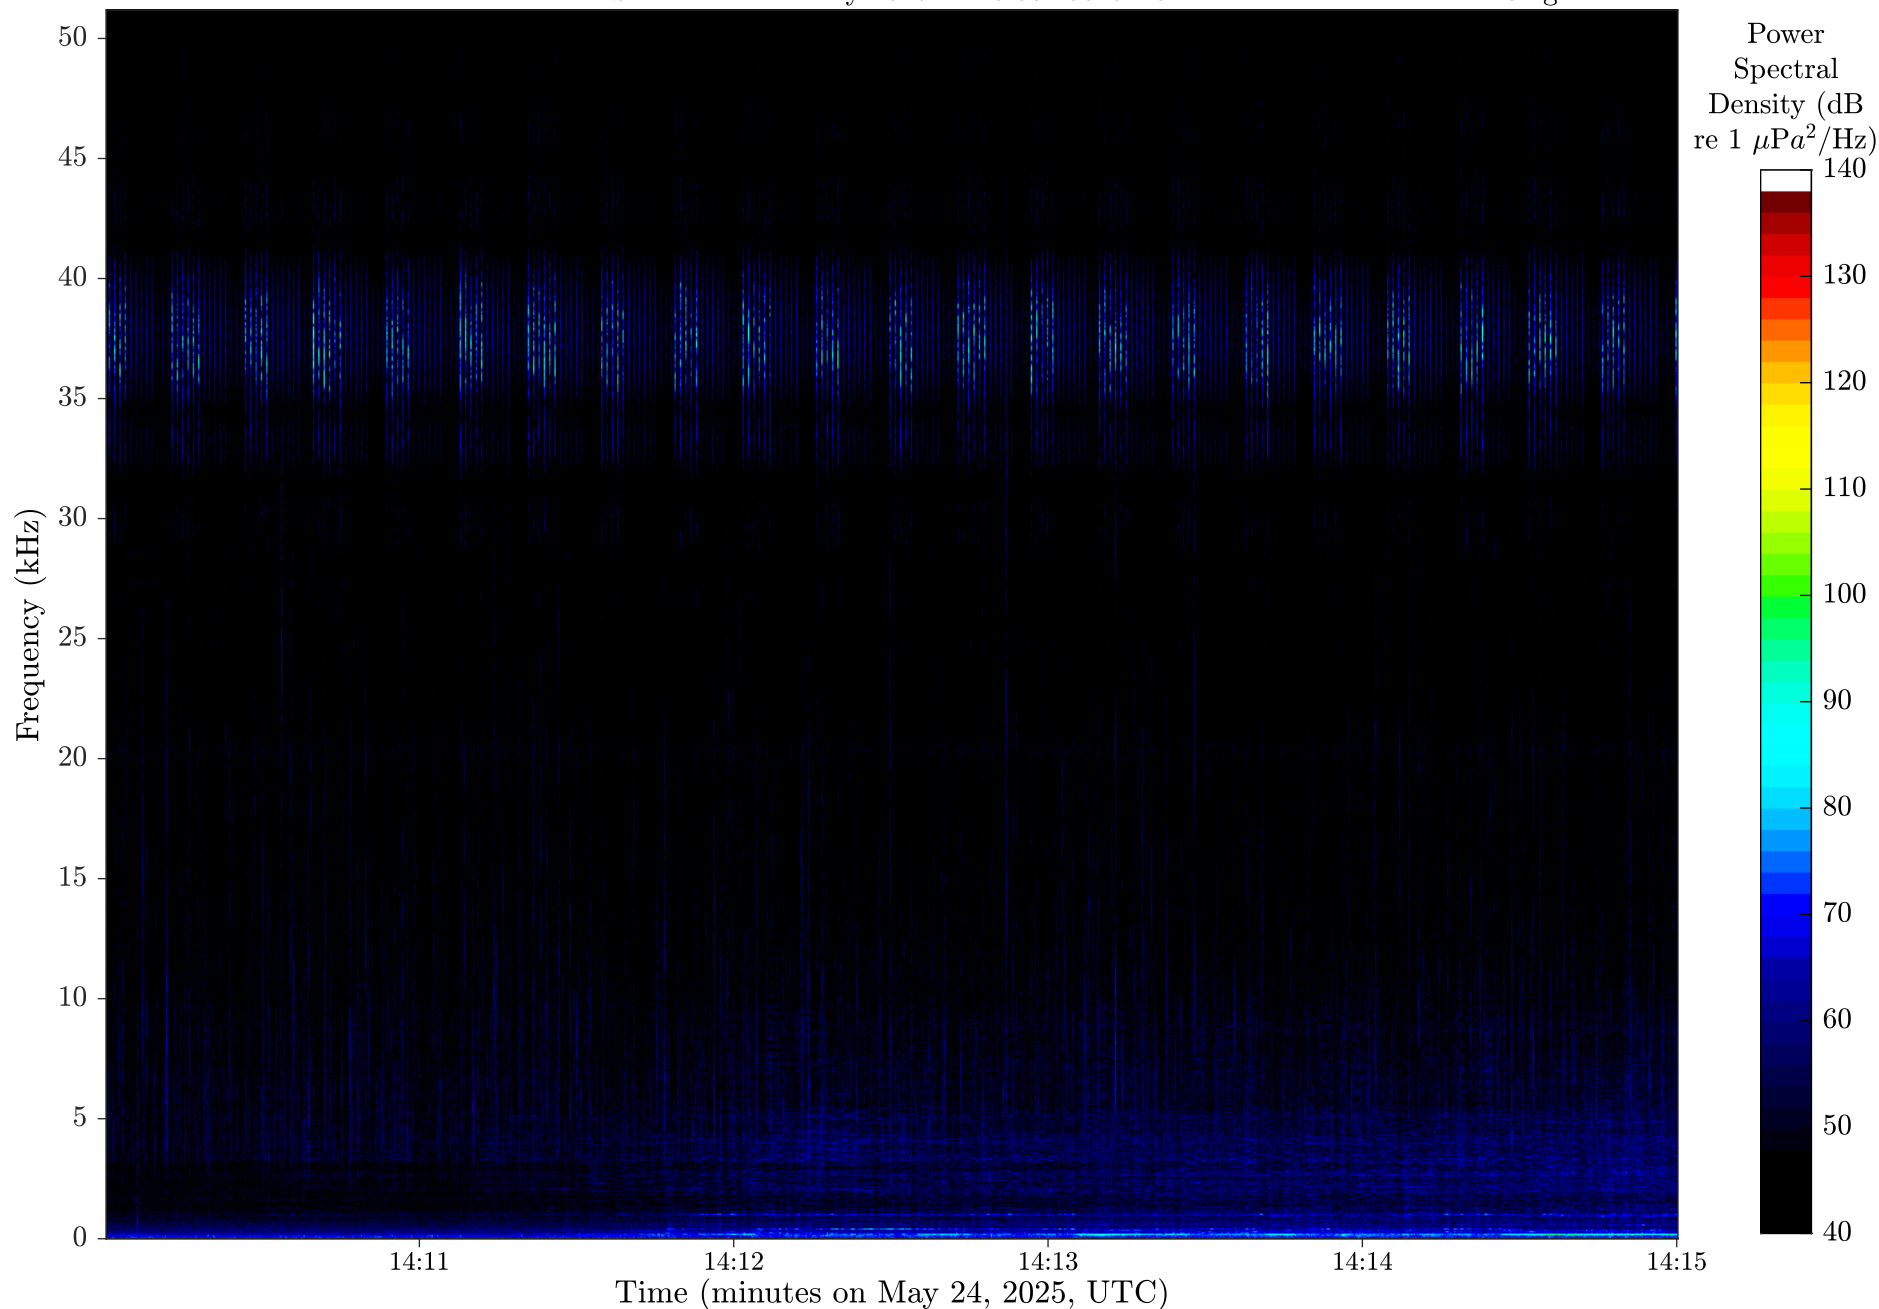


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:30:35 UTC

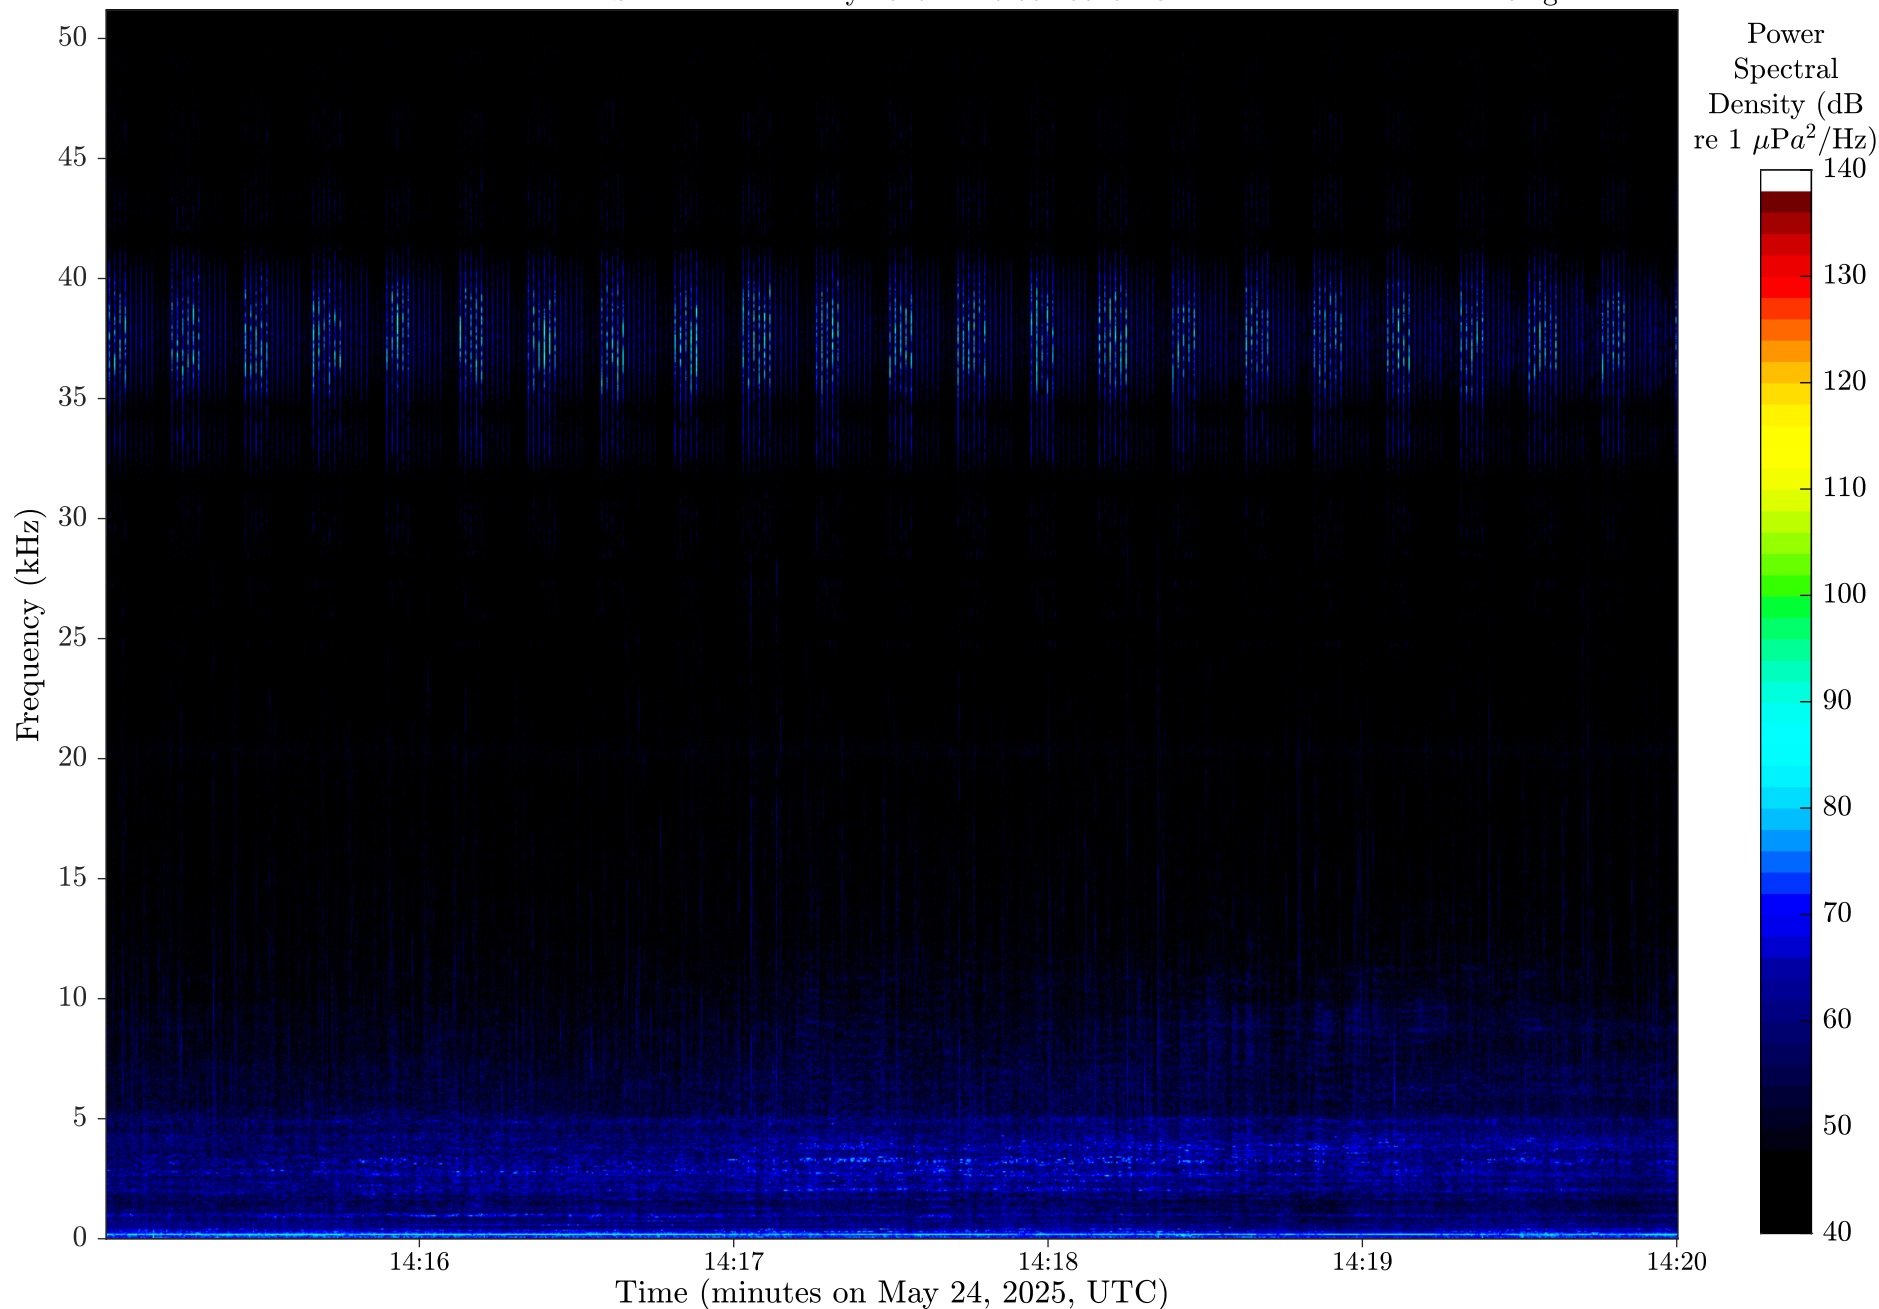

Comments: 31.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:30:43 UTC

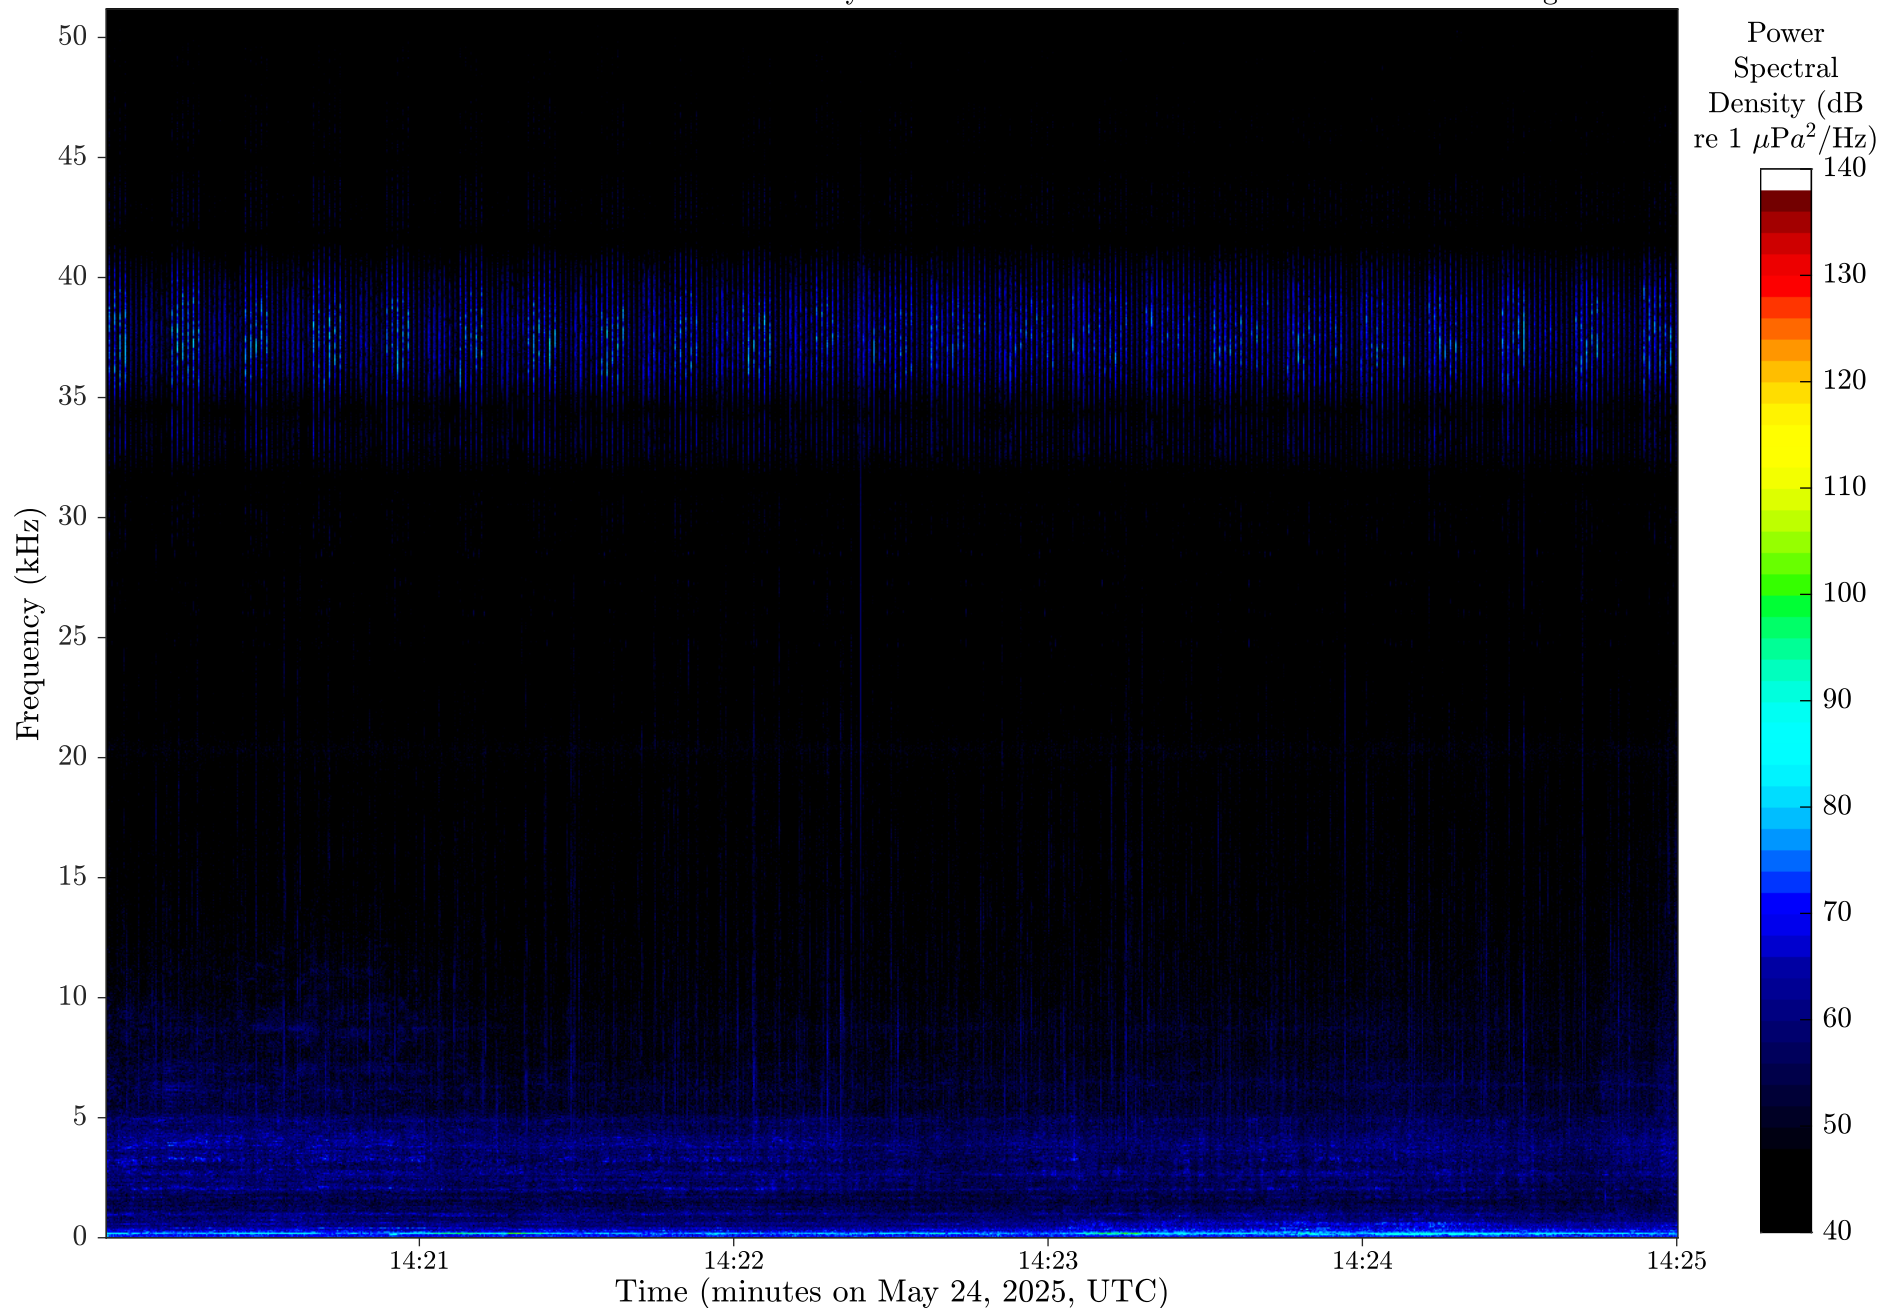

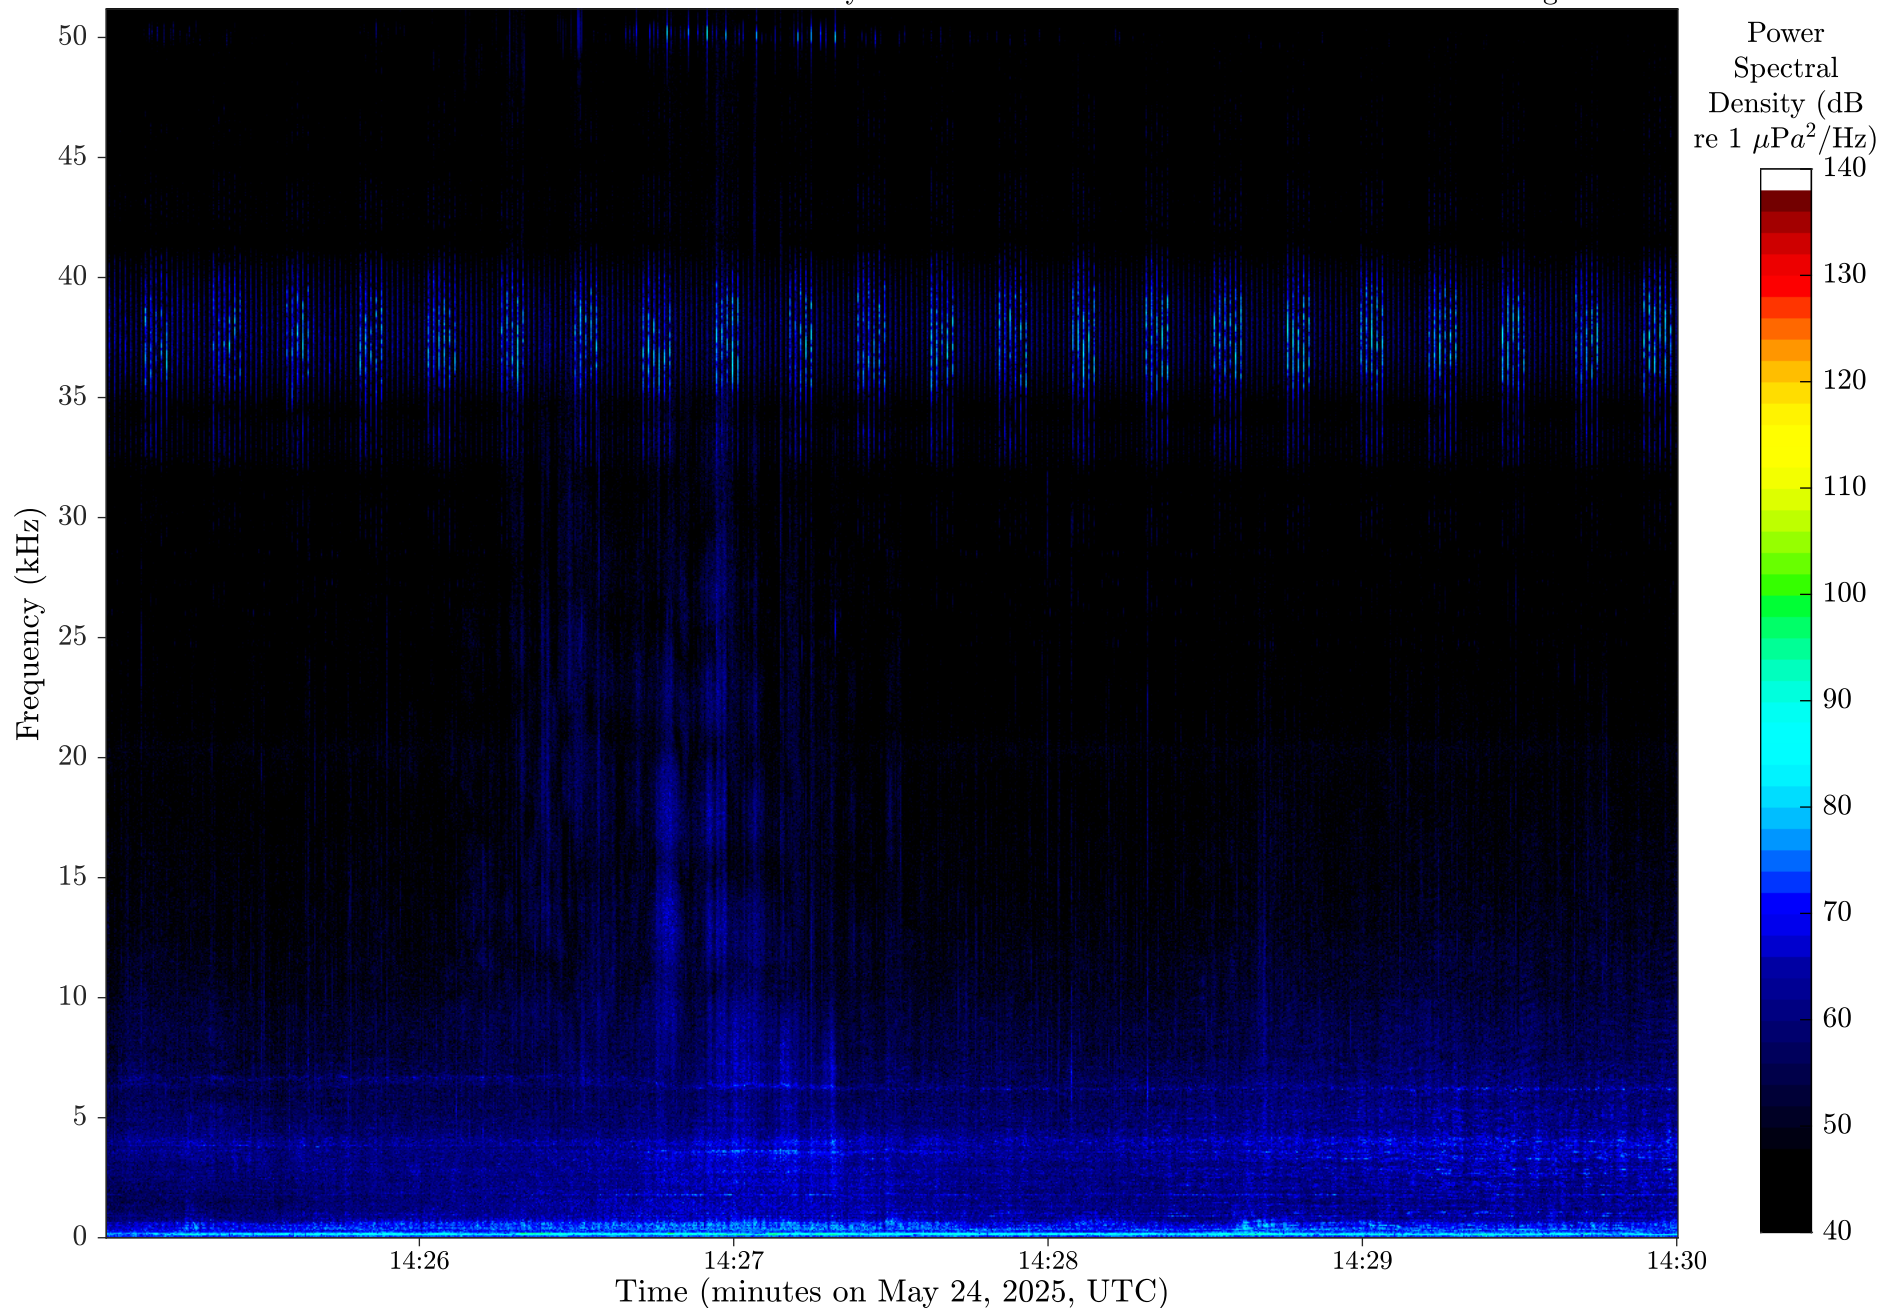


Comments: 20.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:00 UTC

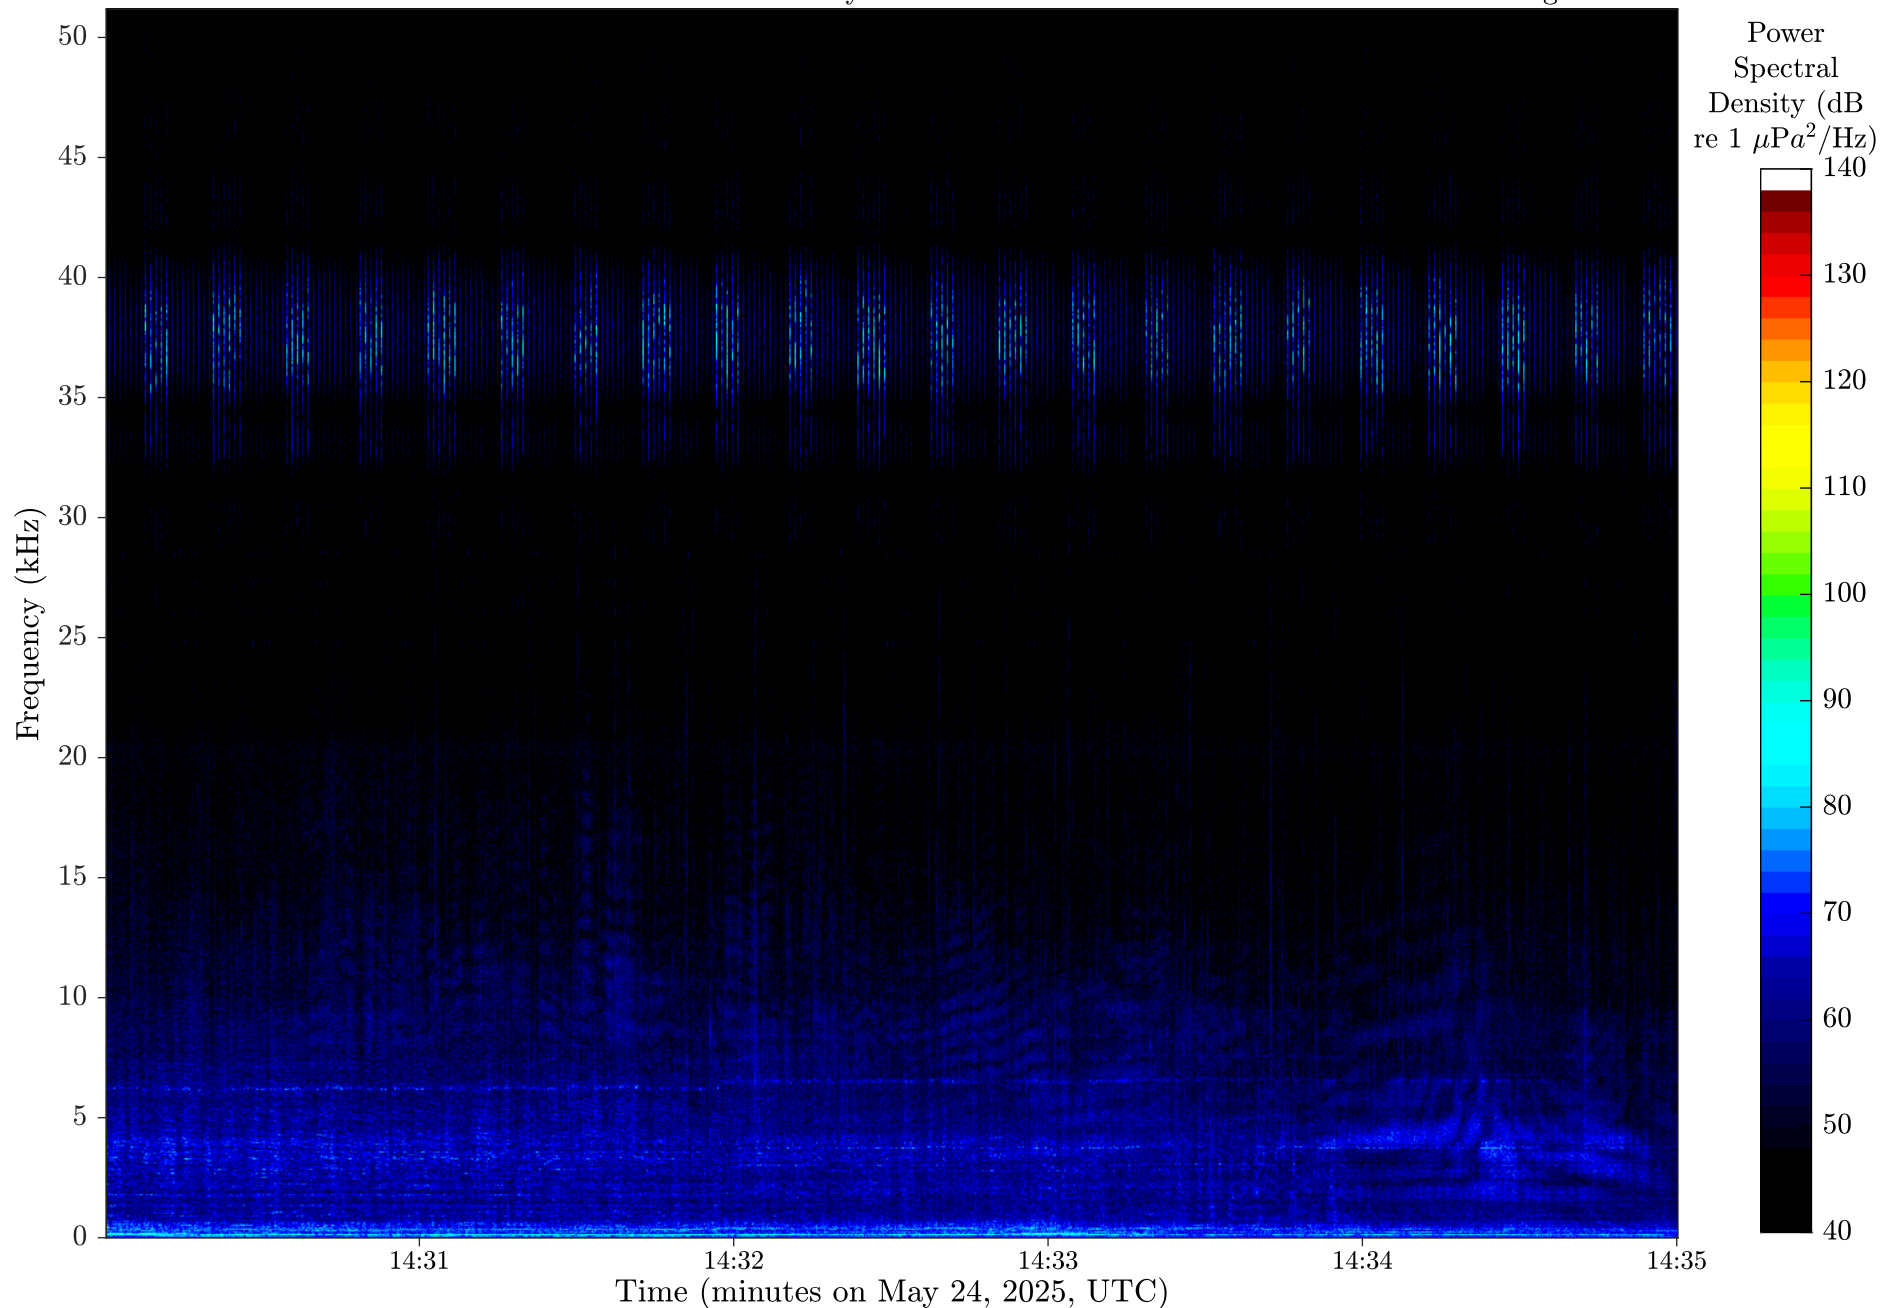


Comments: 27.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:08 UTC

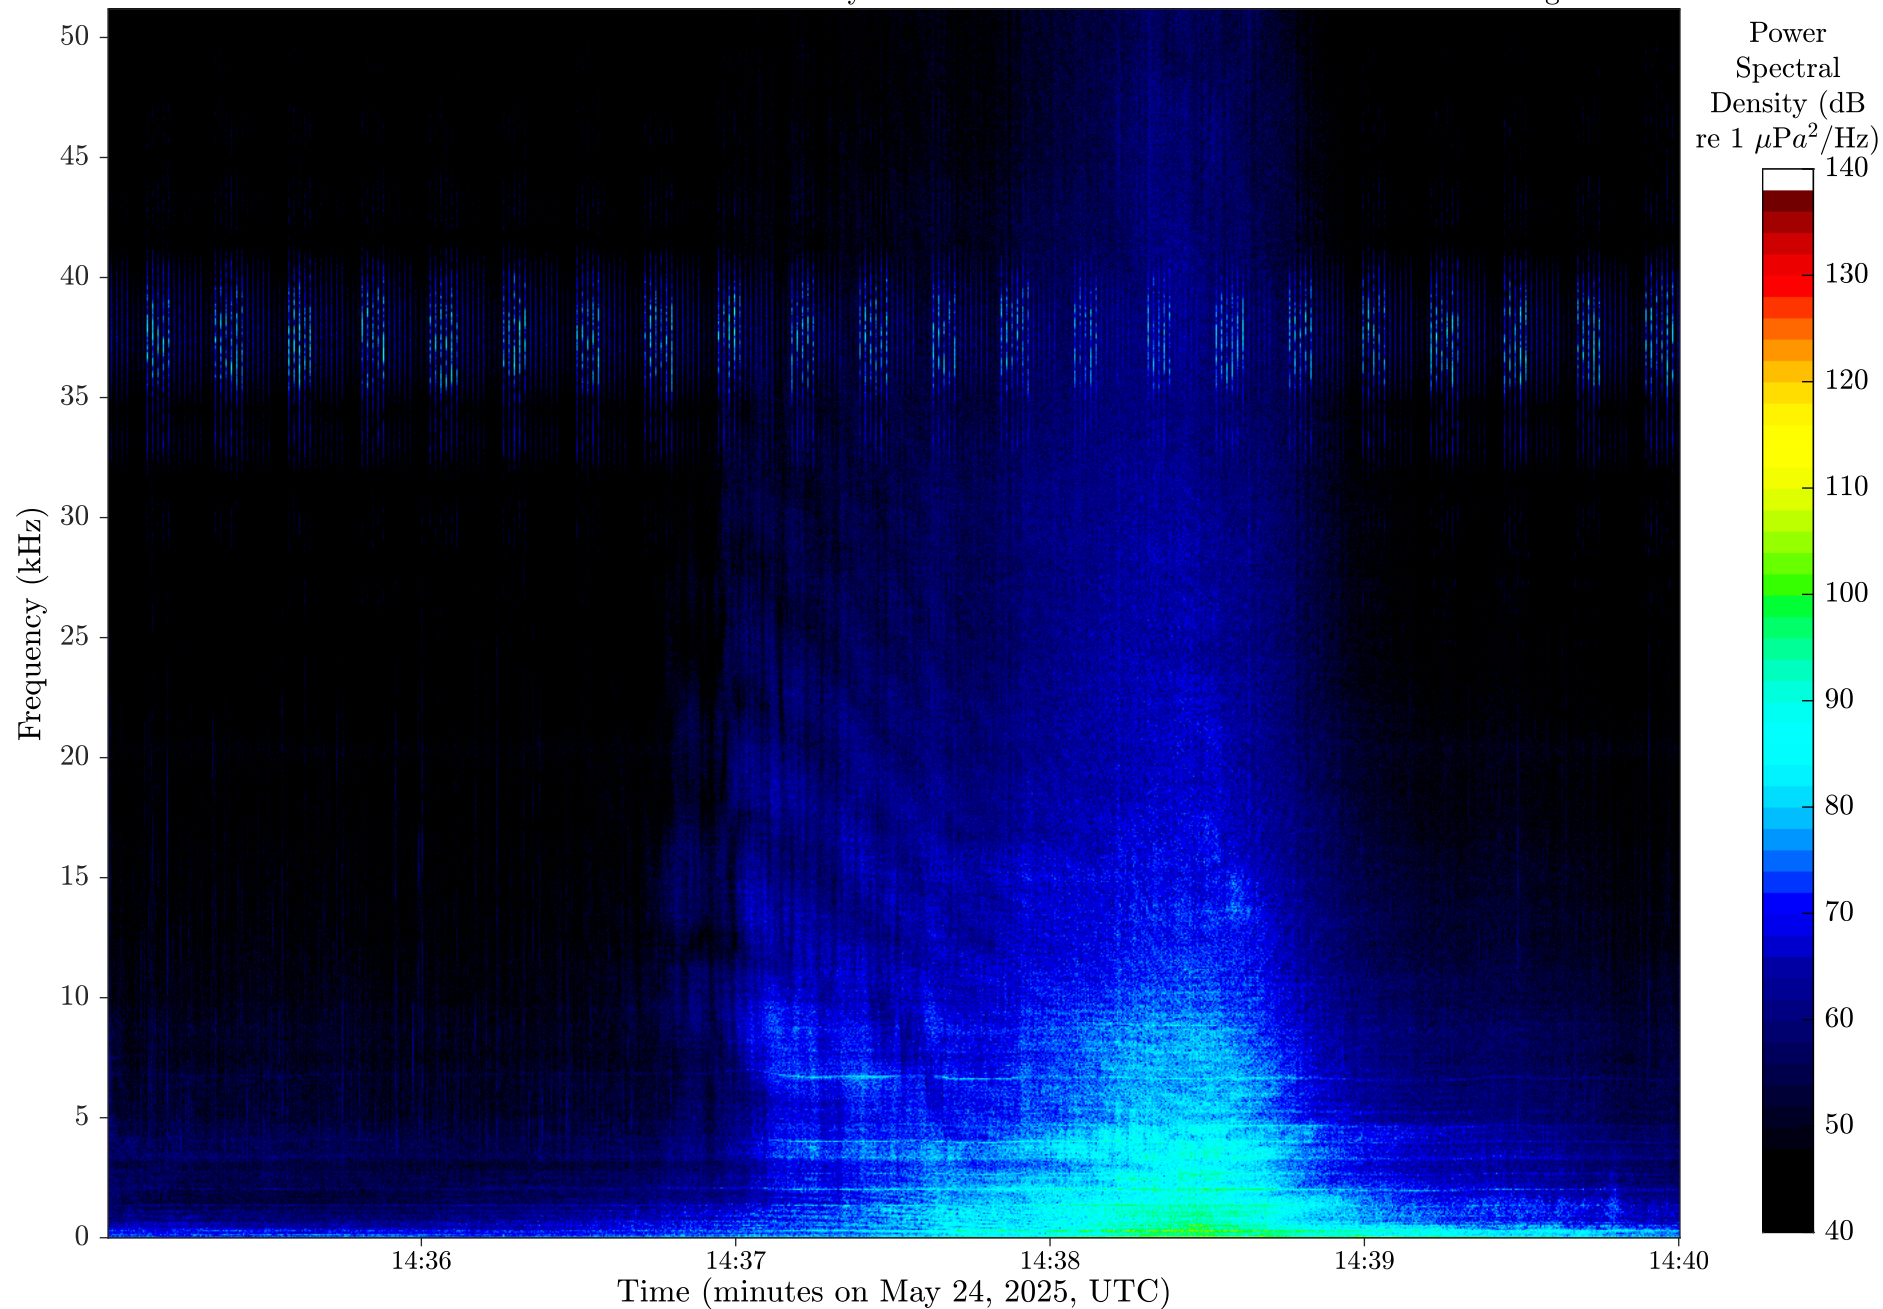


Comments: 15 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:16 UTC

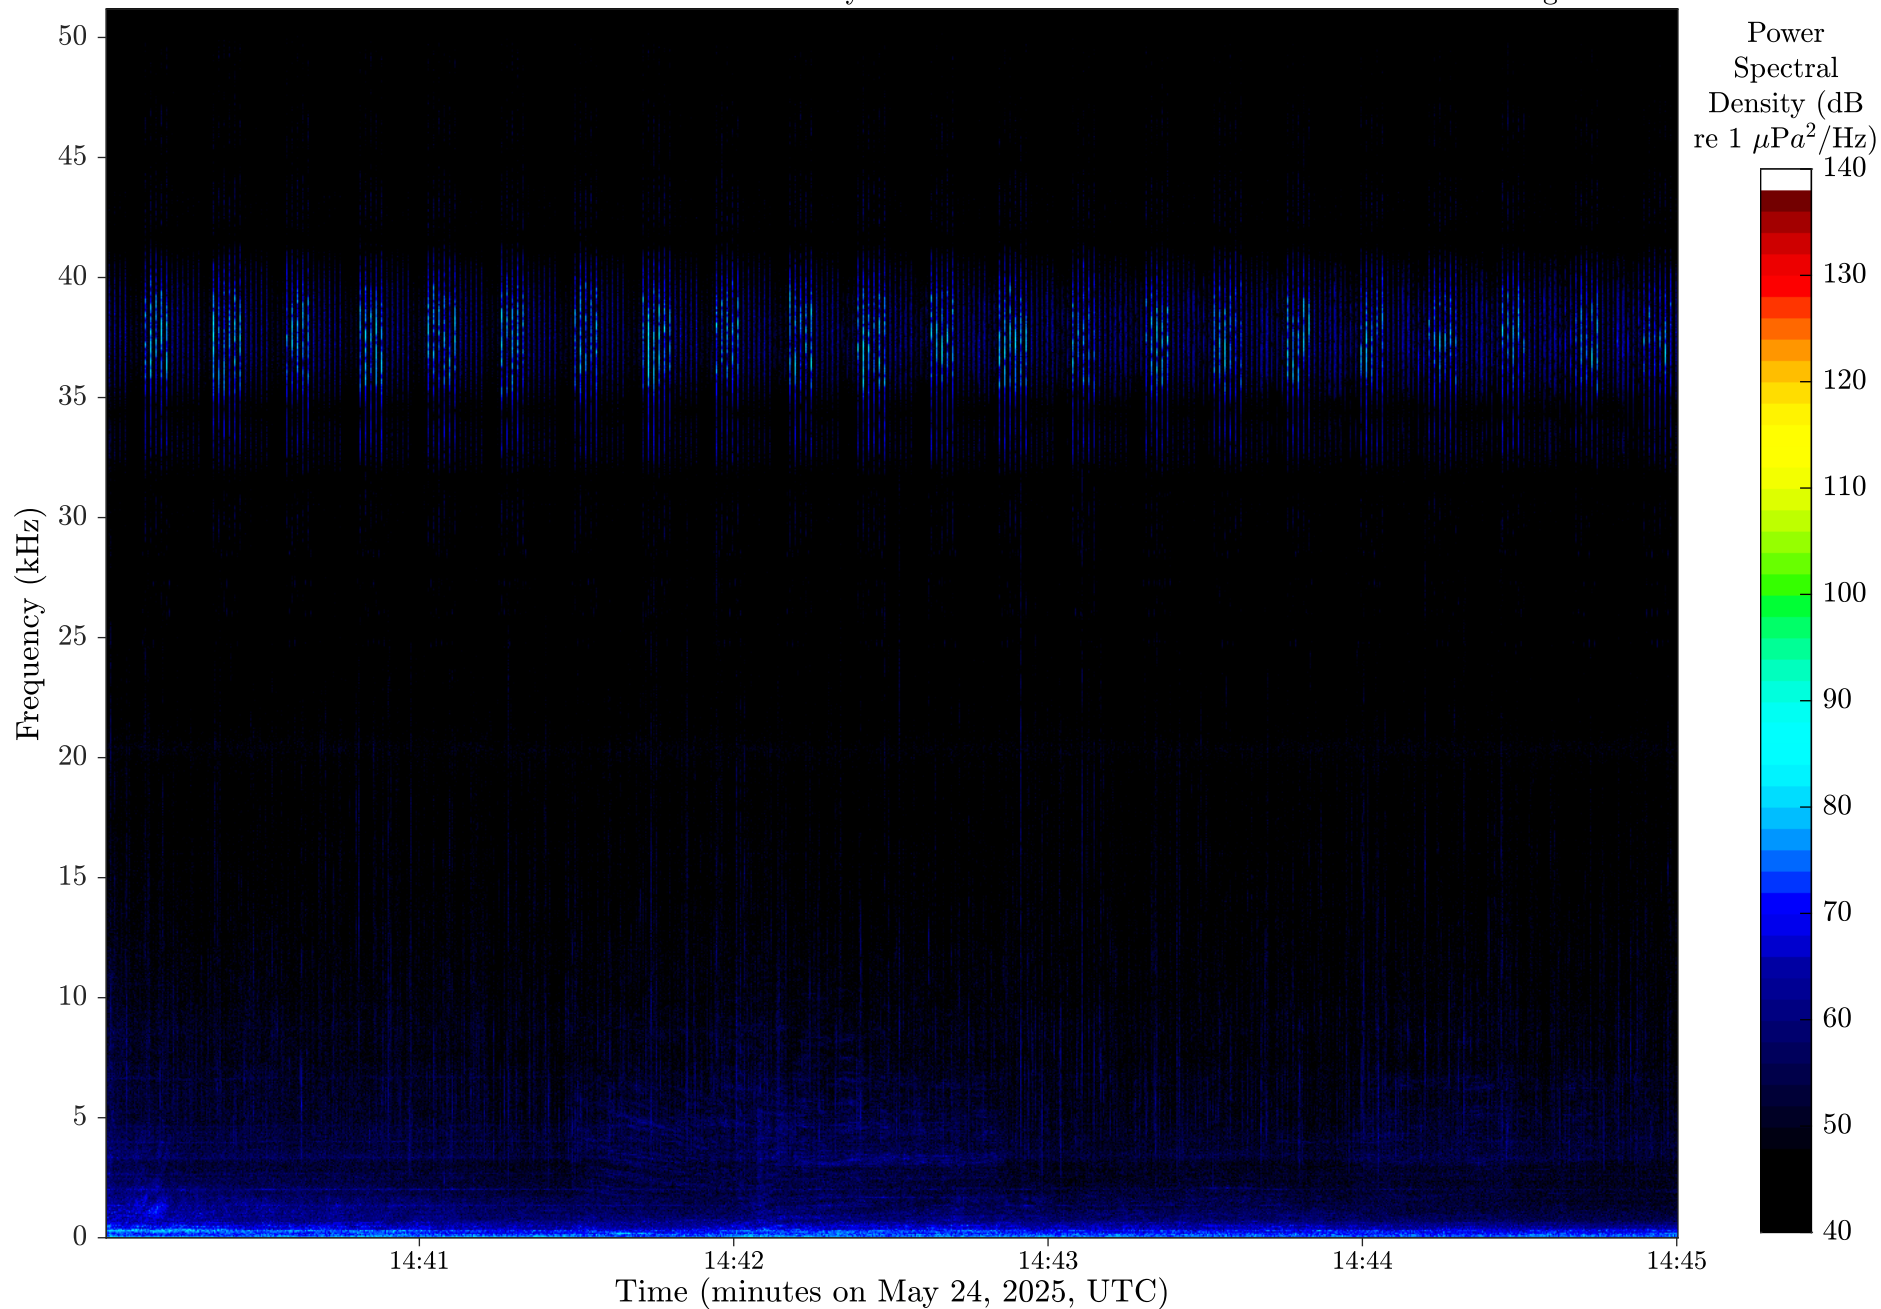


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:24 UTC

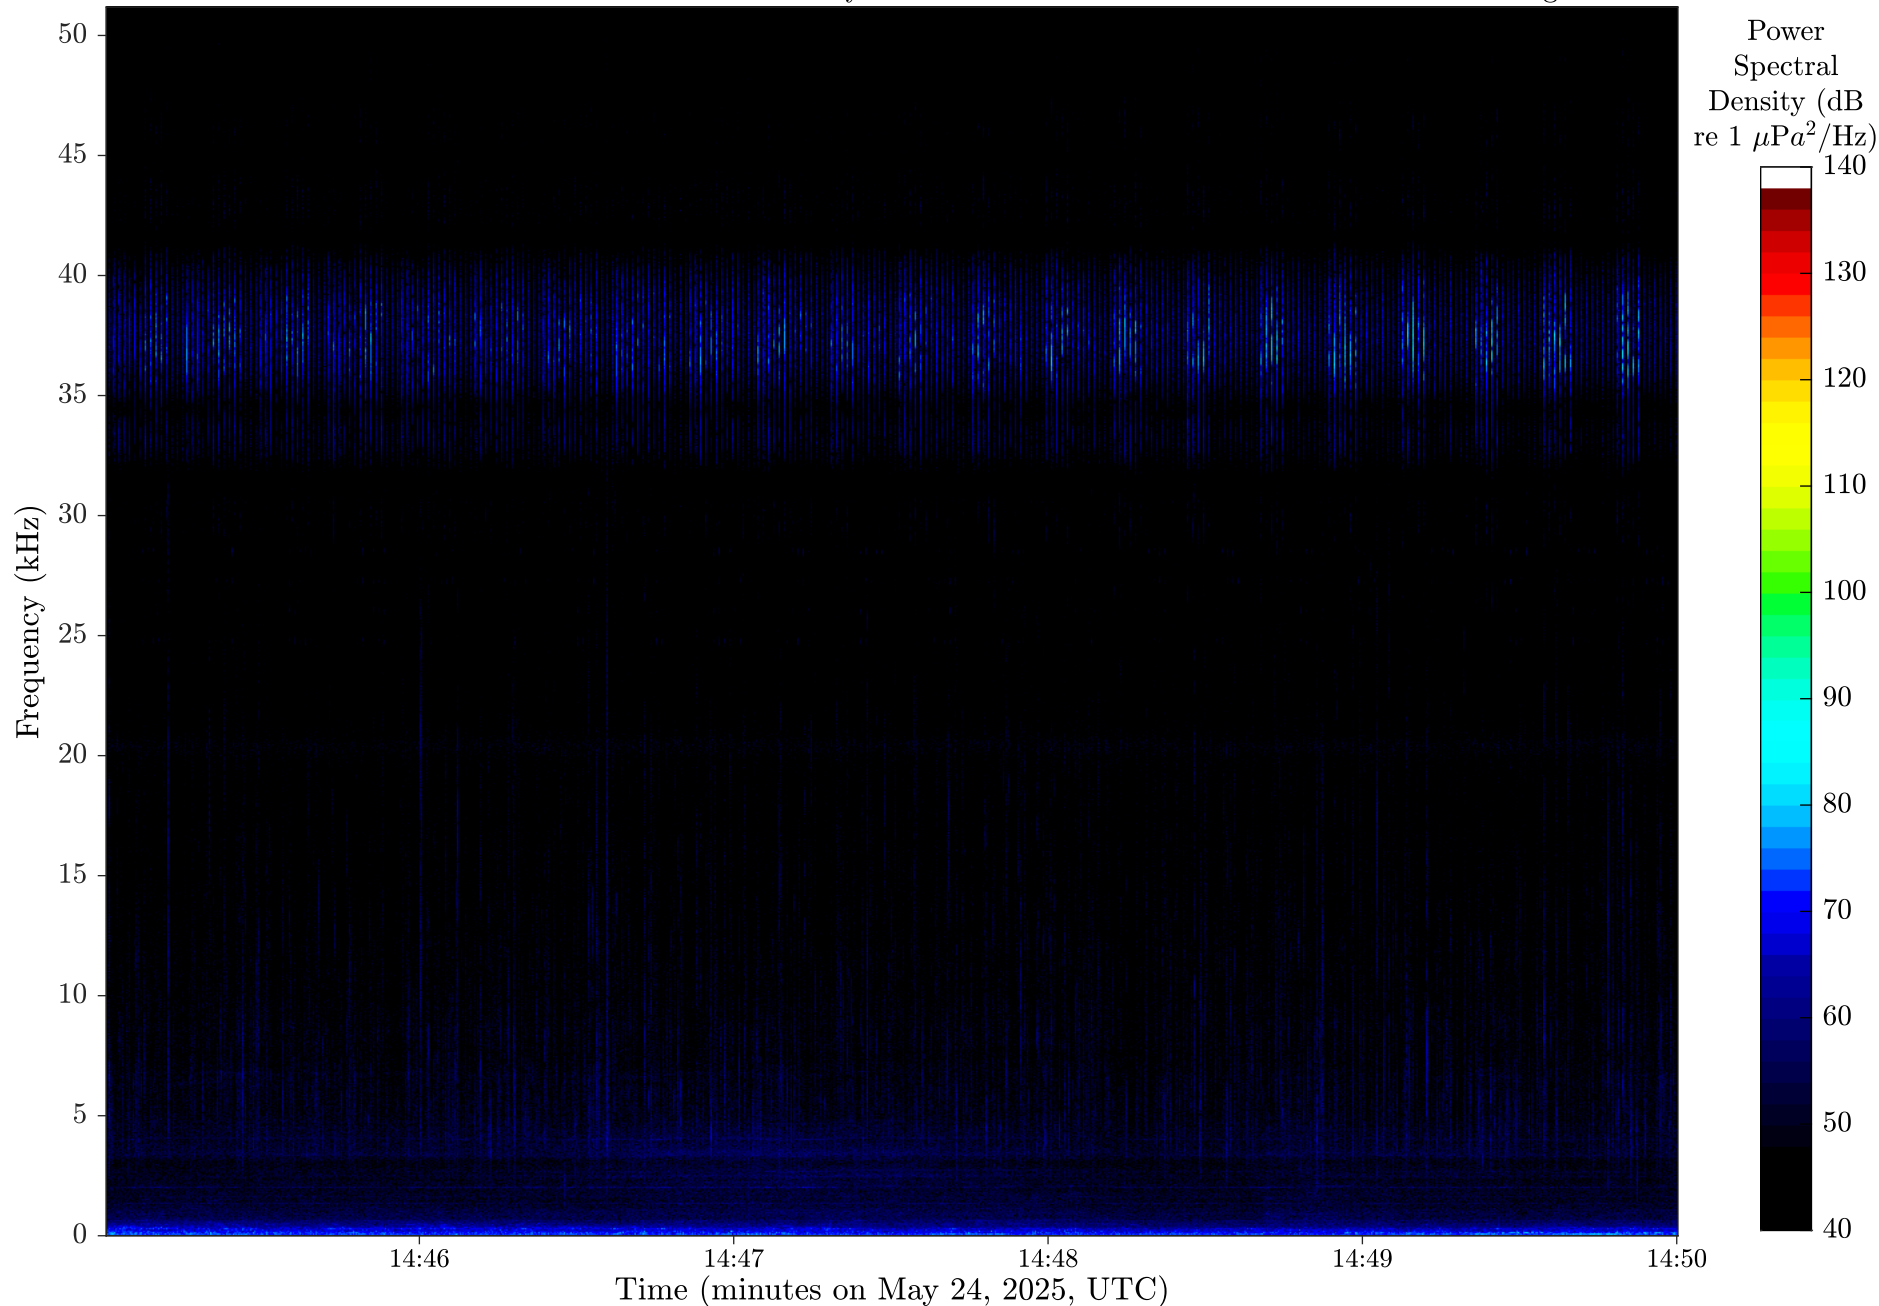


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:31 UTC

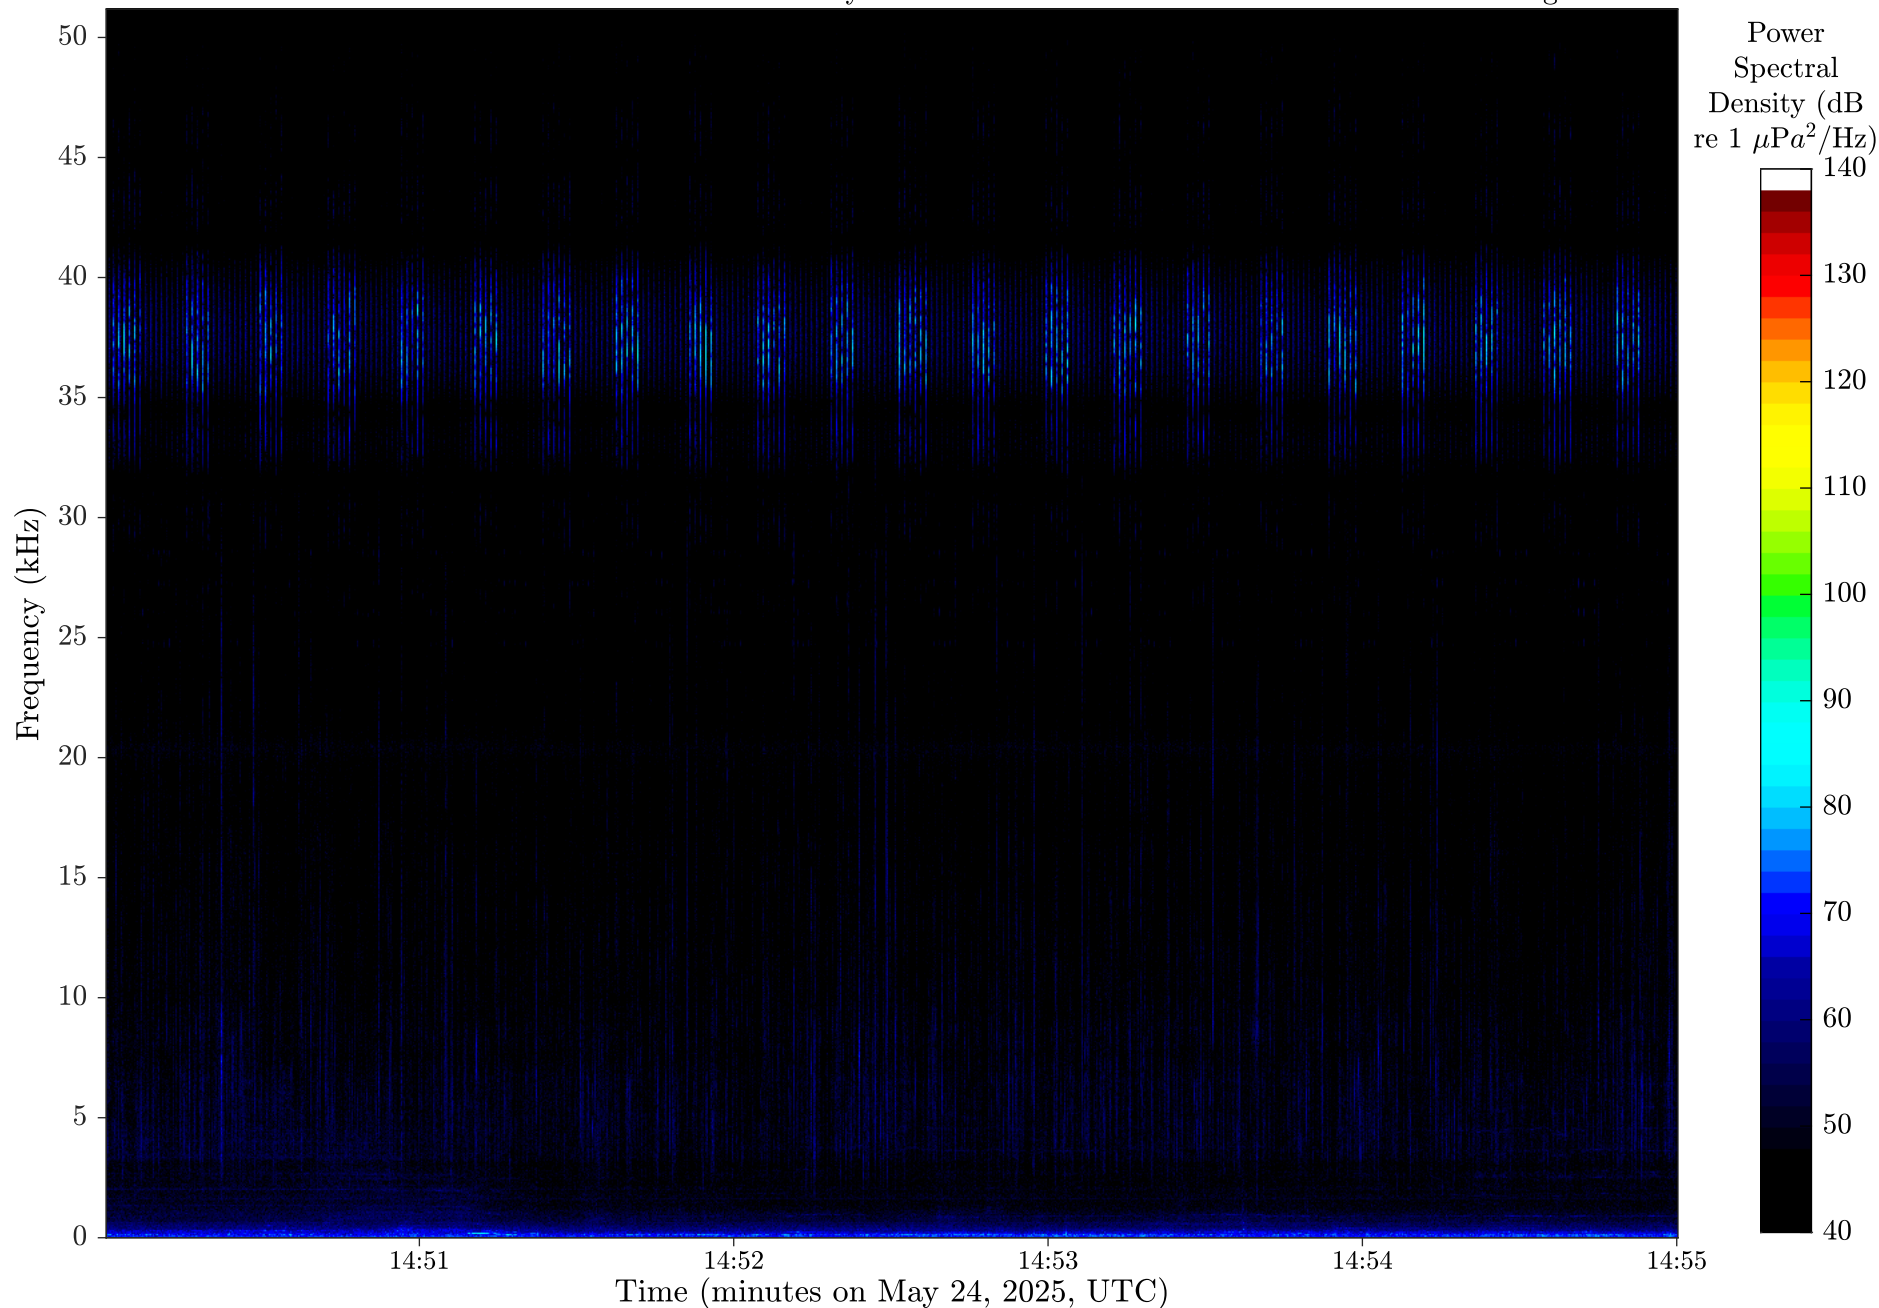


Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:39 UTC

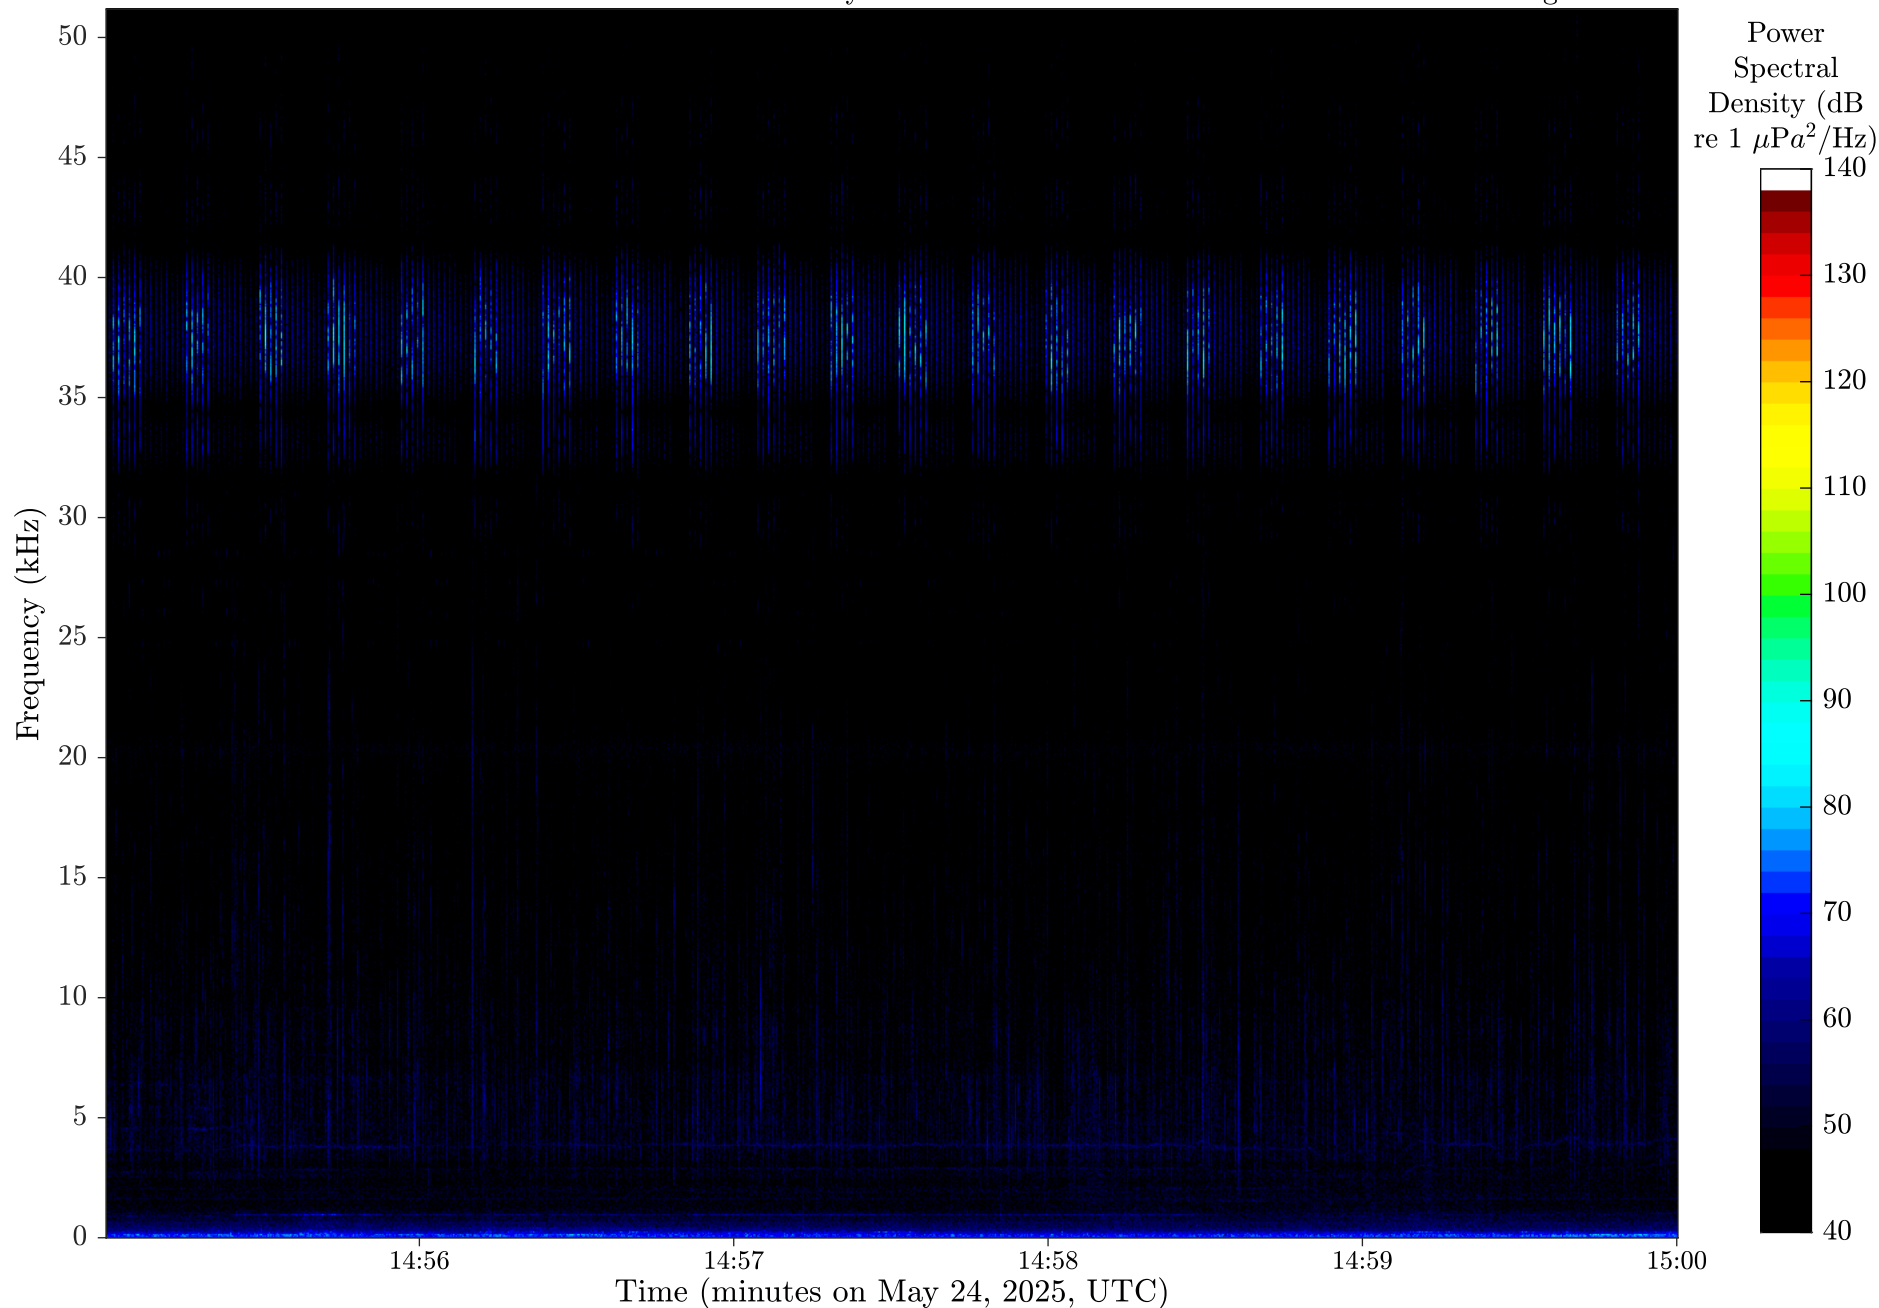


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:46 UTC

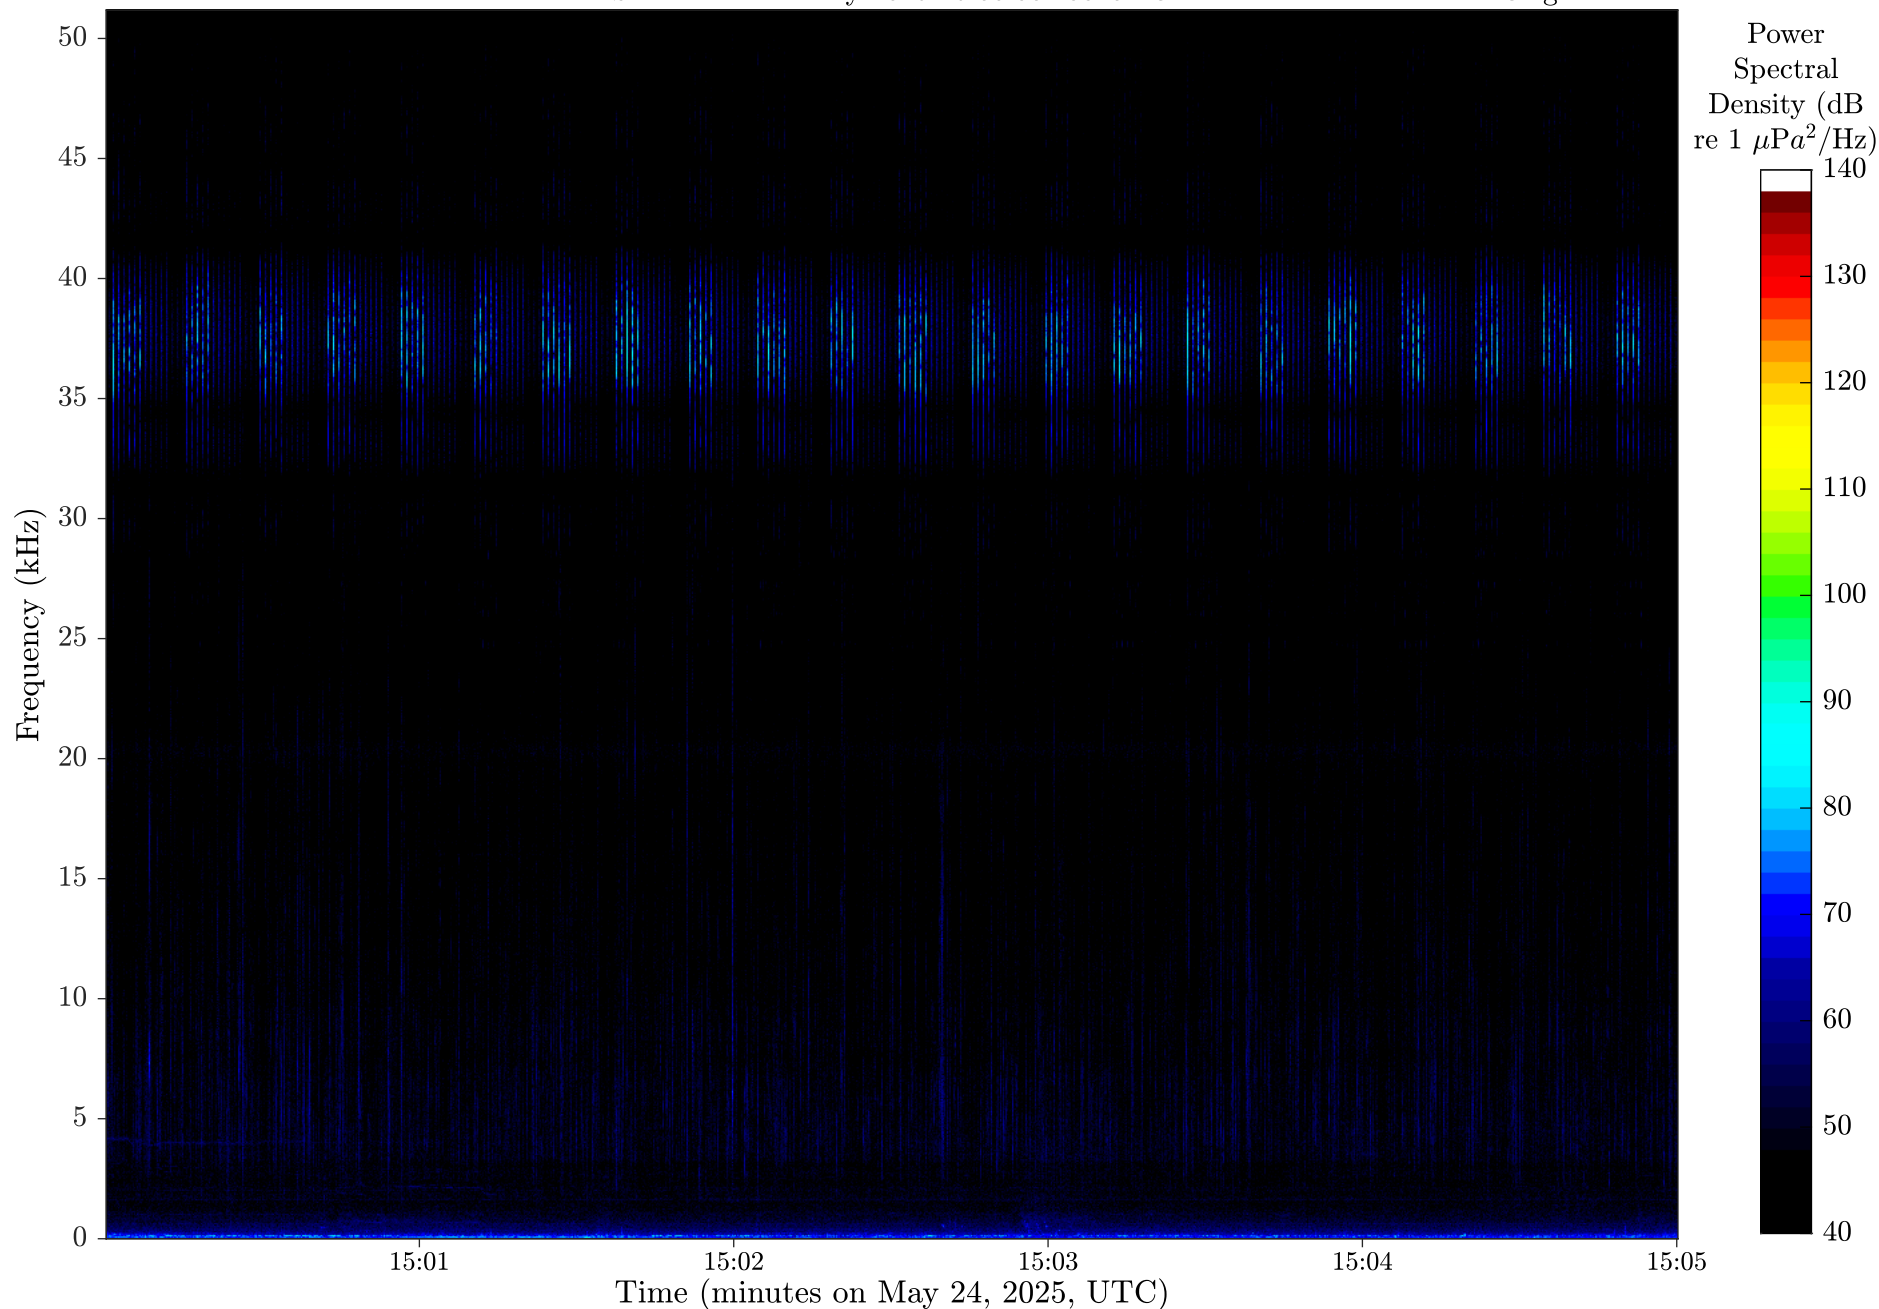


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:54 UTC

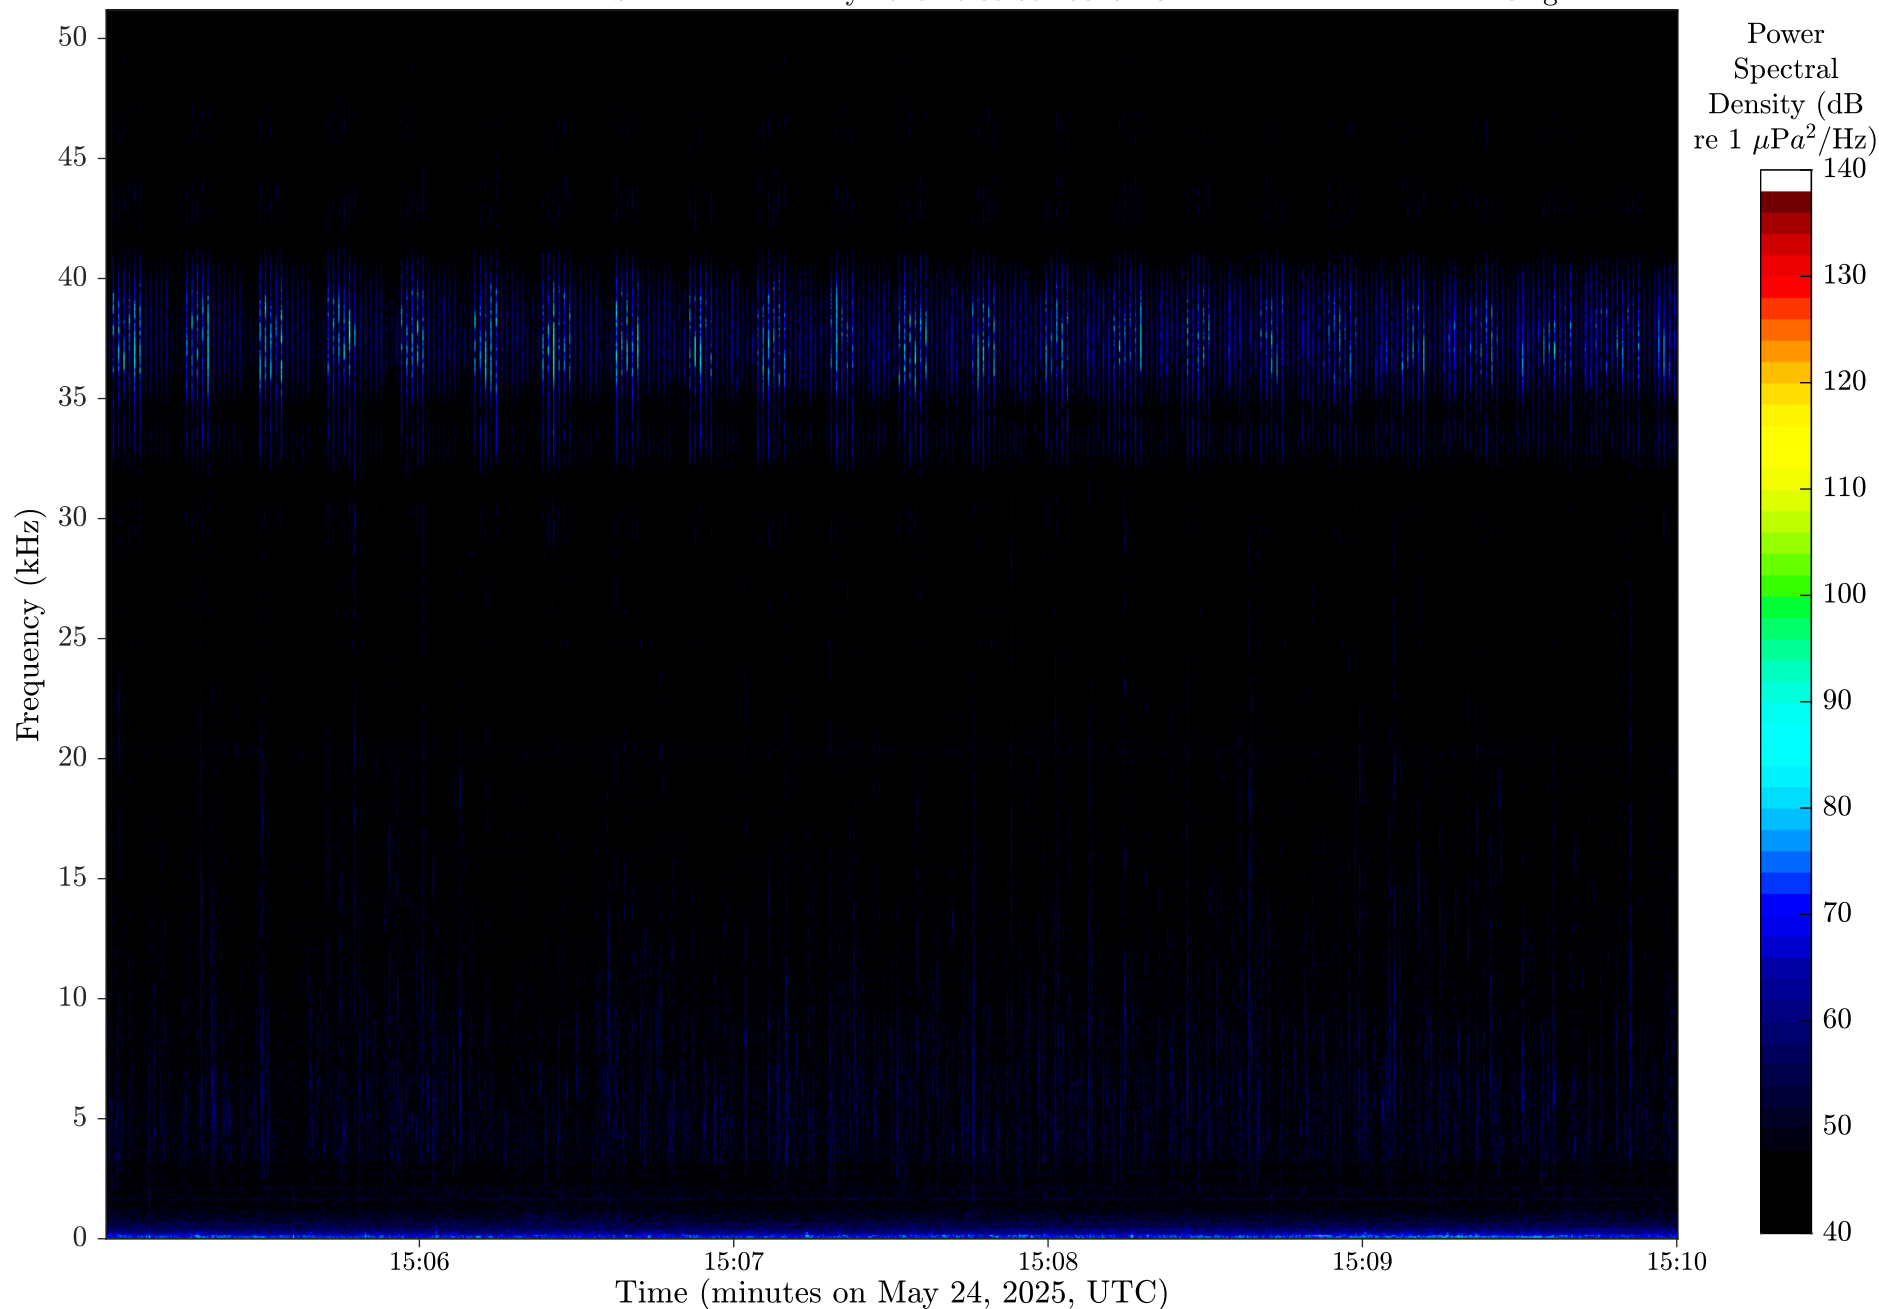


Comments: 32.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:32:01 UTC

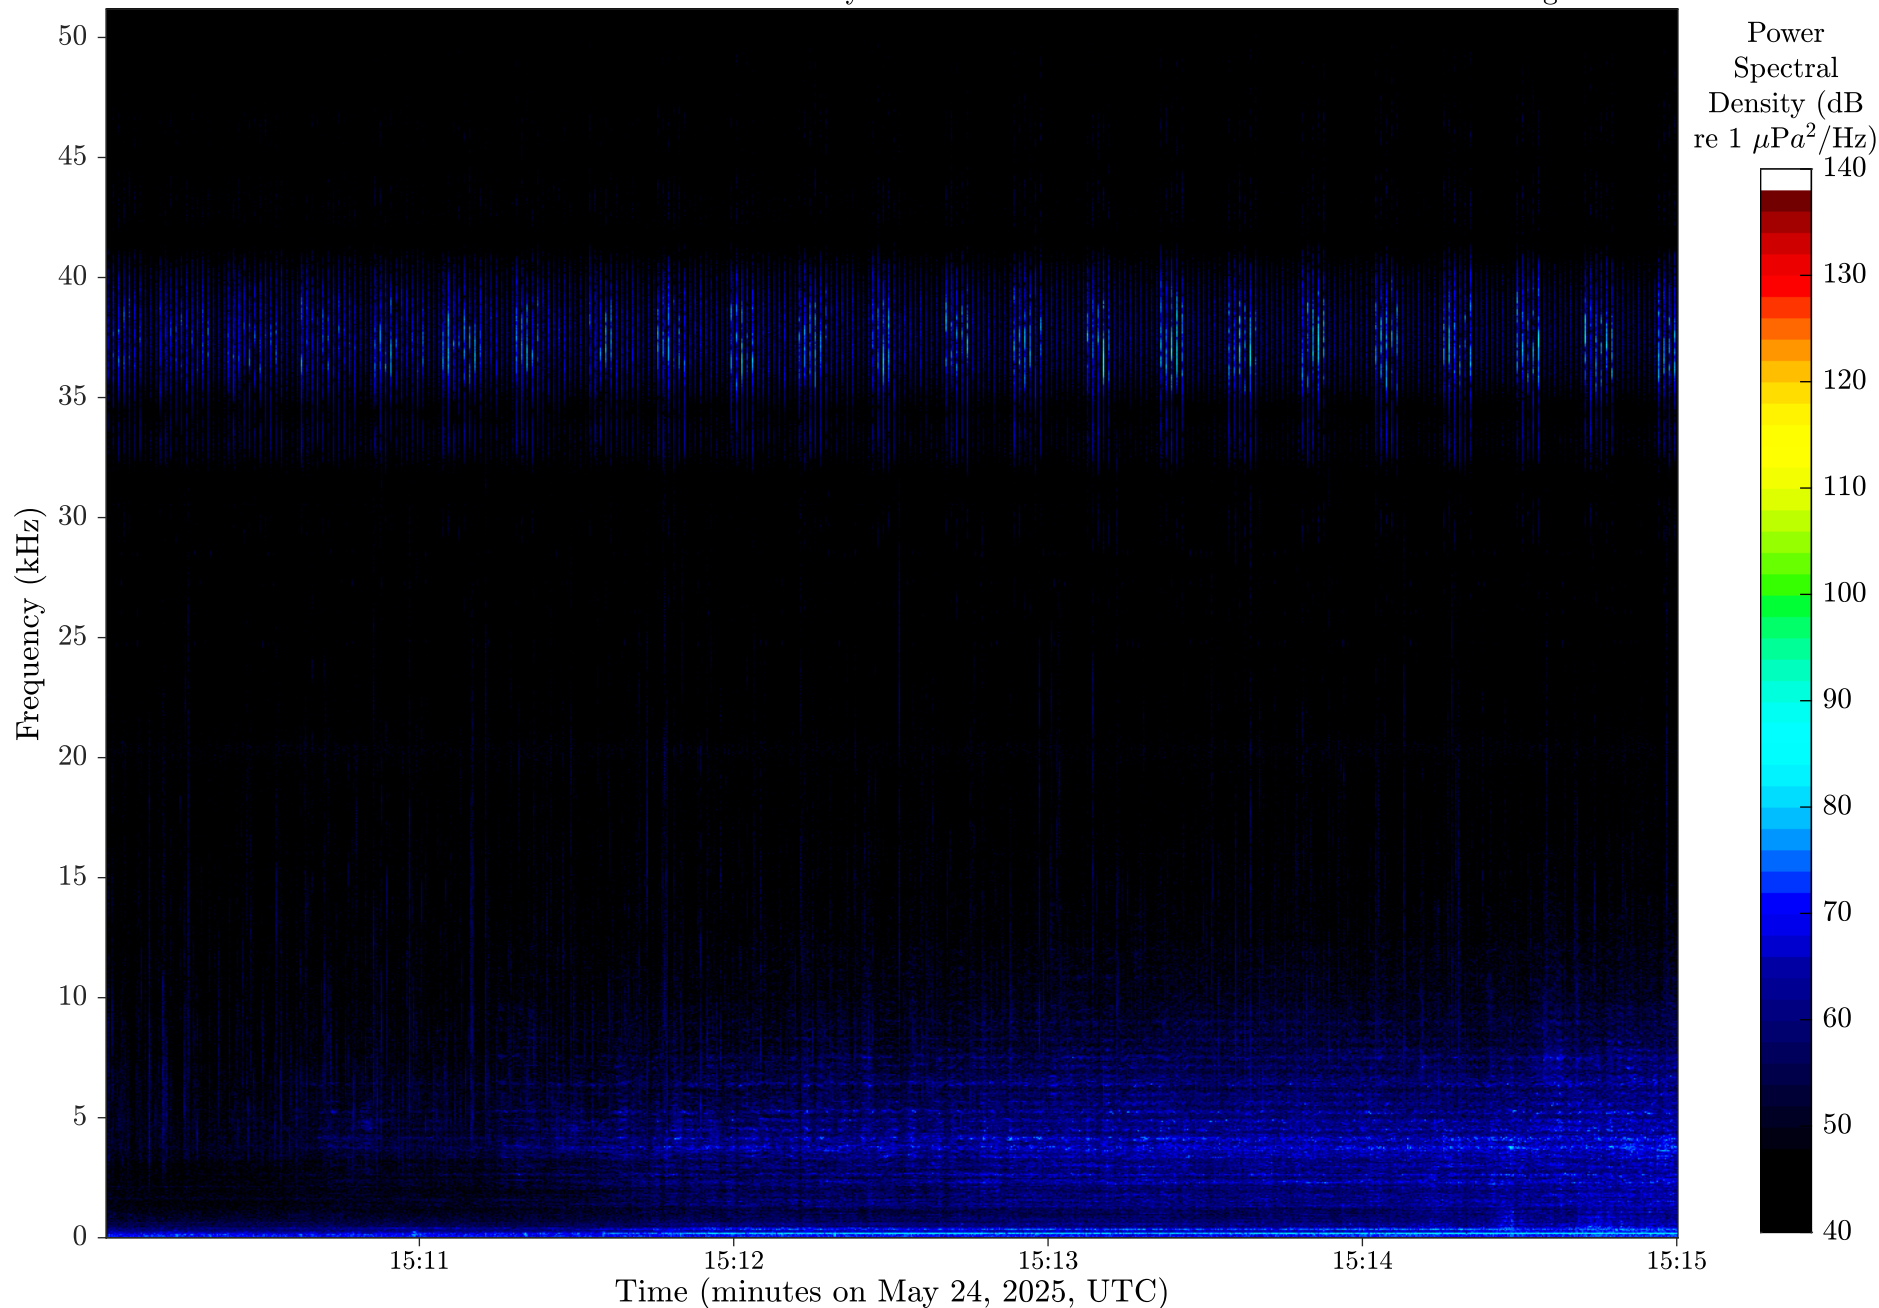


Comments: 31.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:32:10 UTC

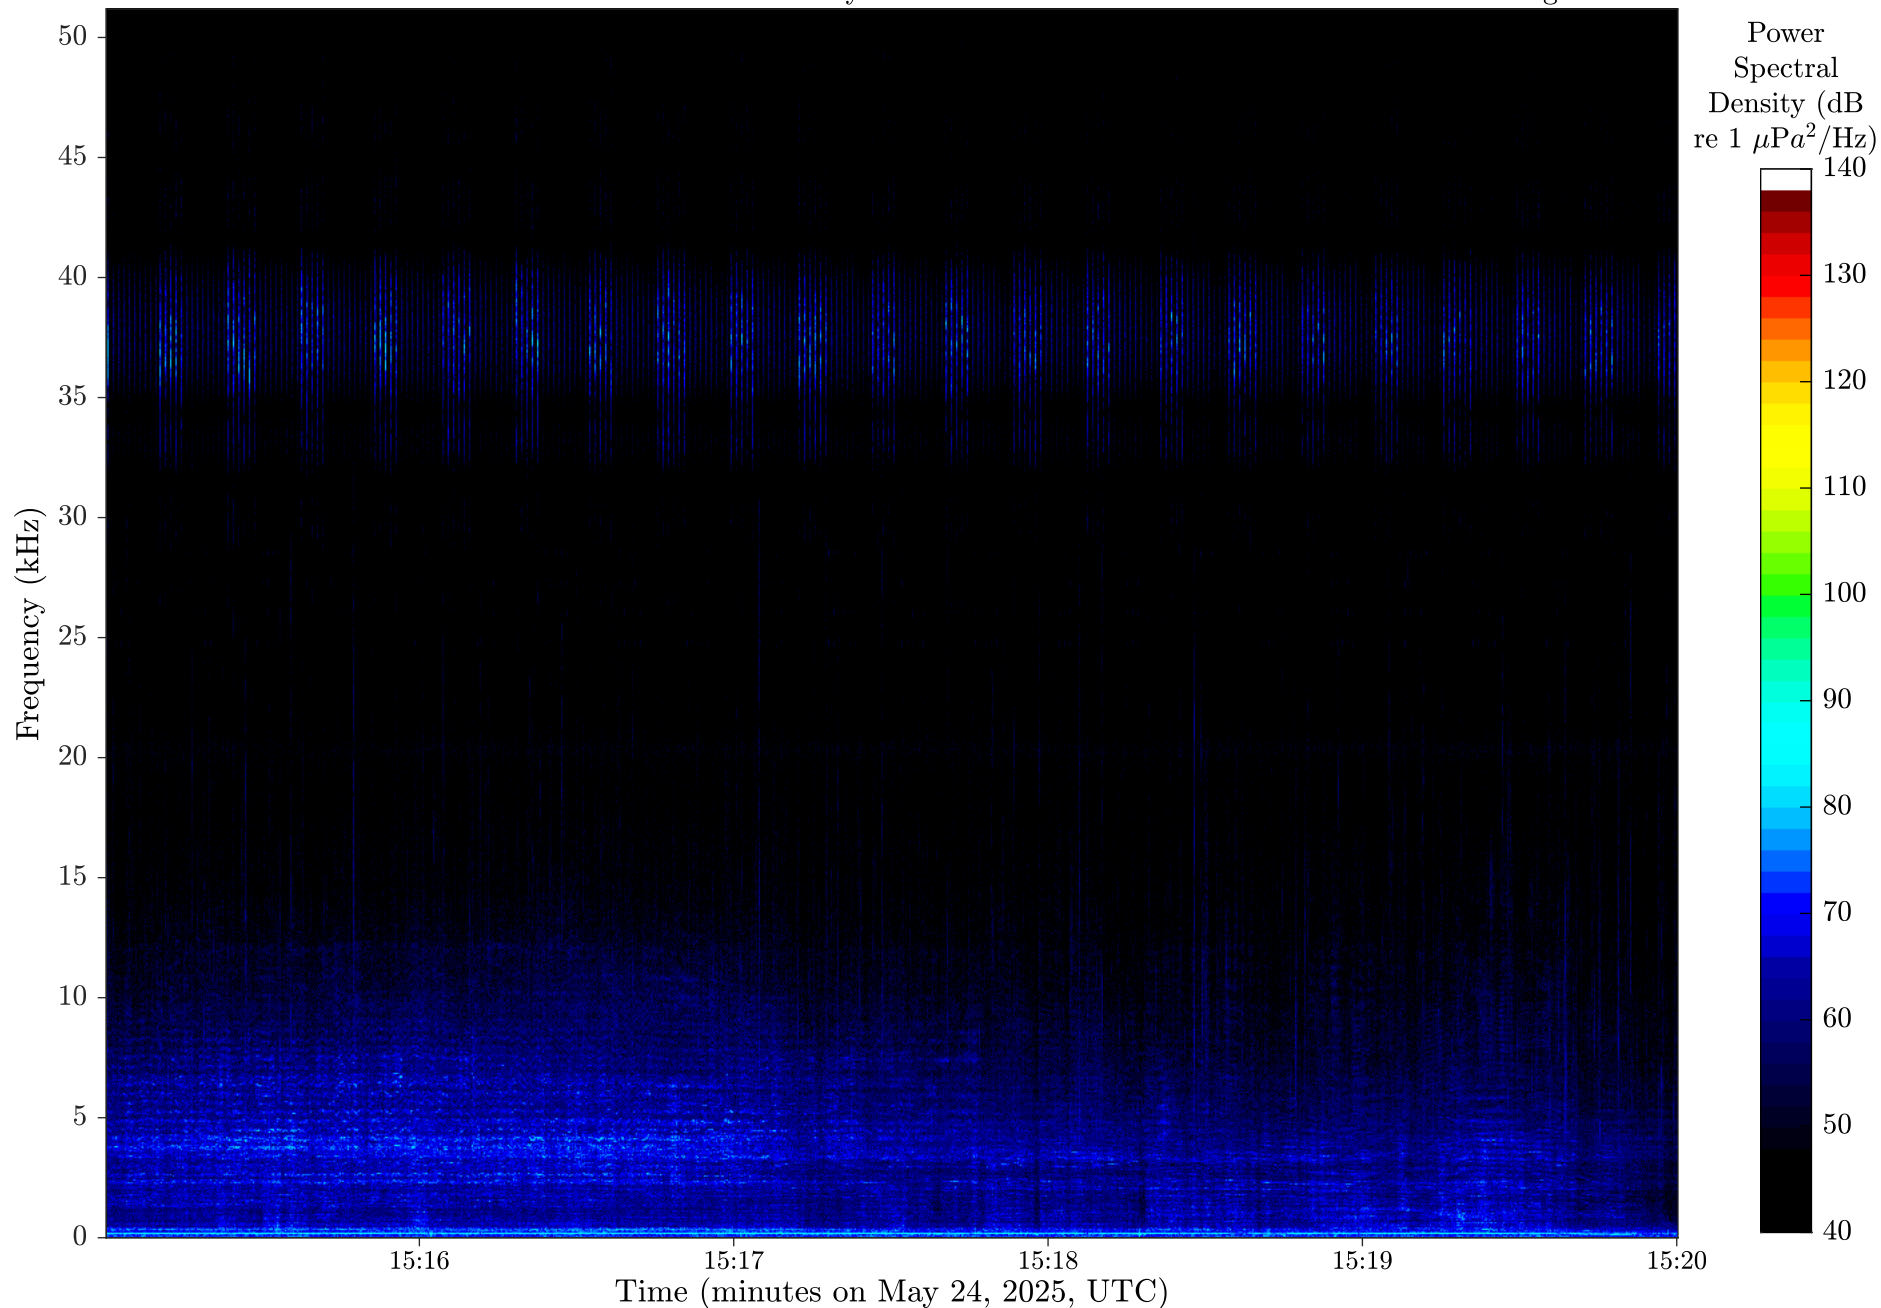


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:32:18 UTC

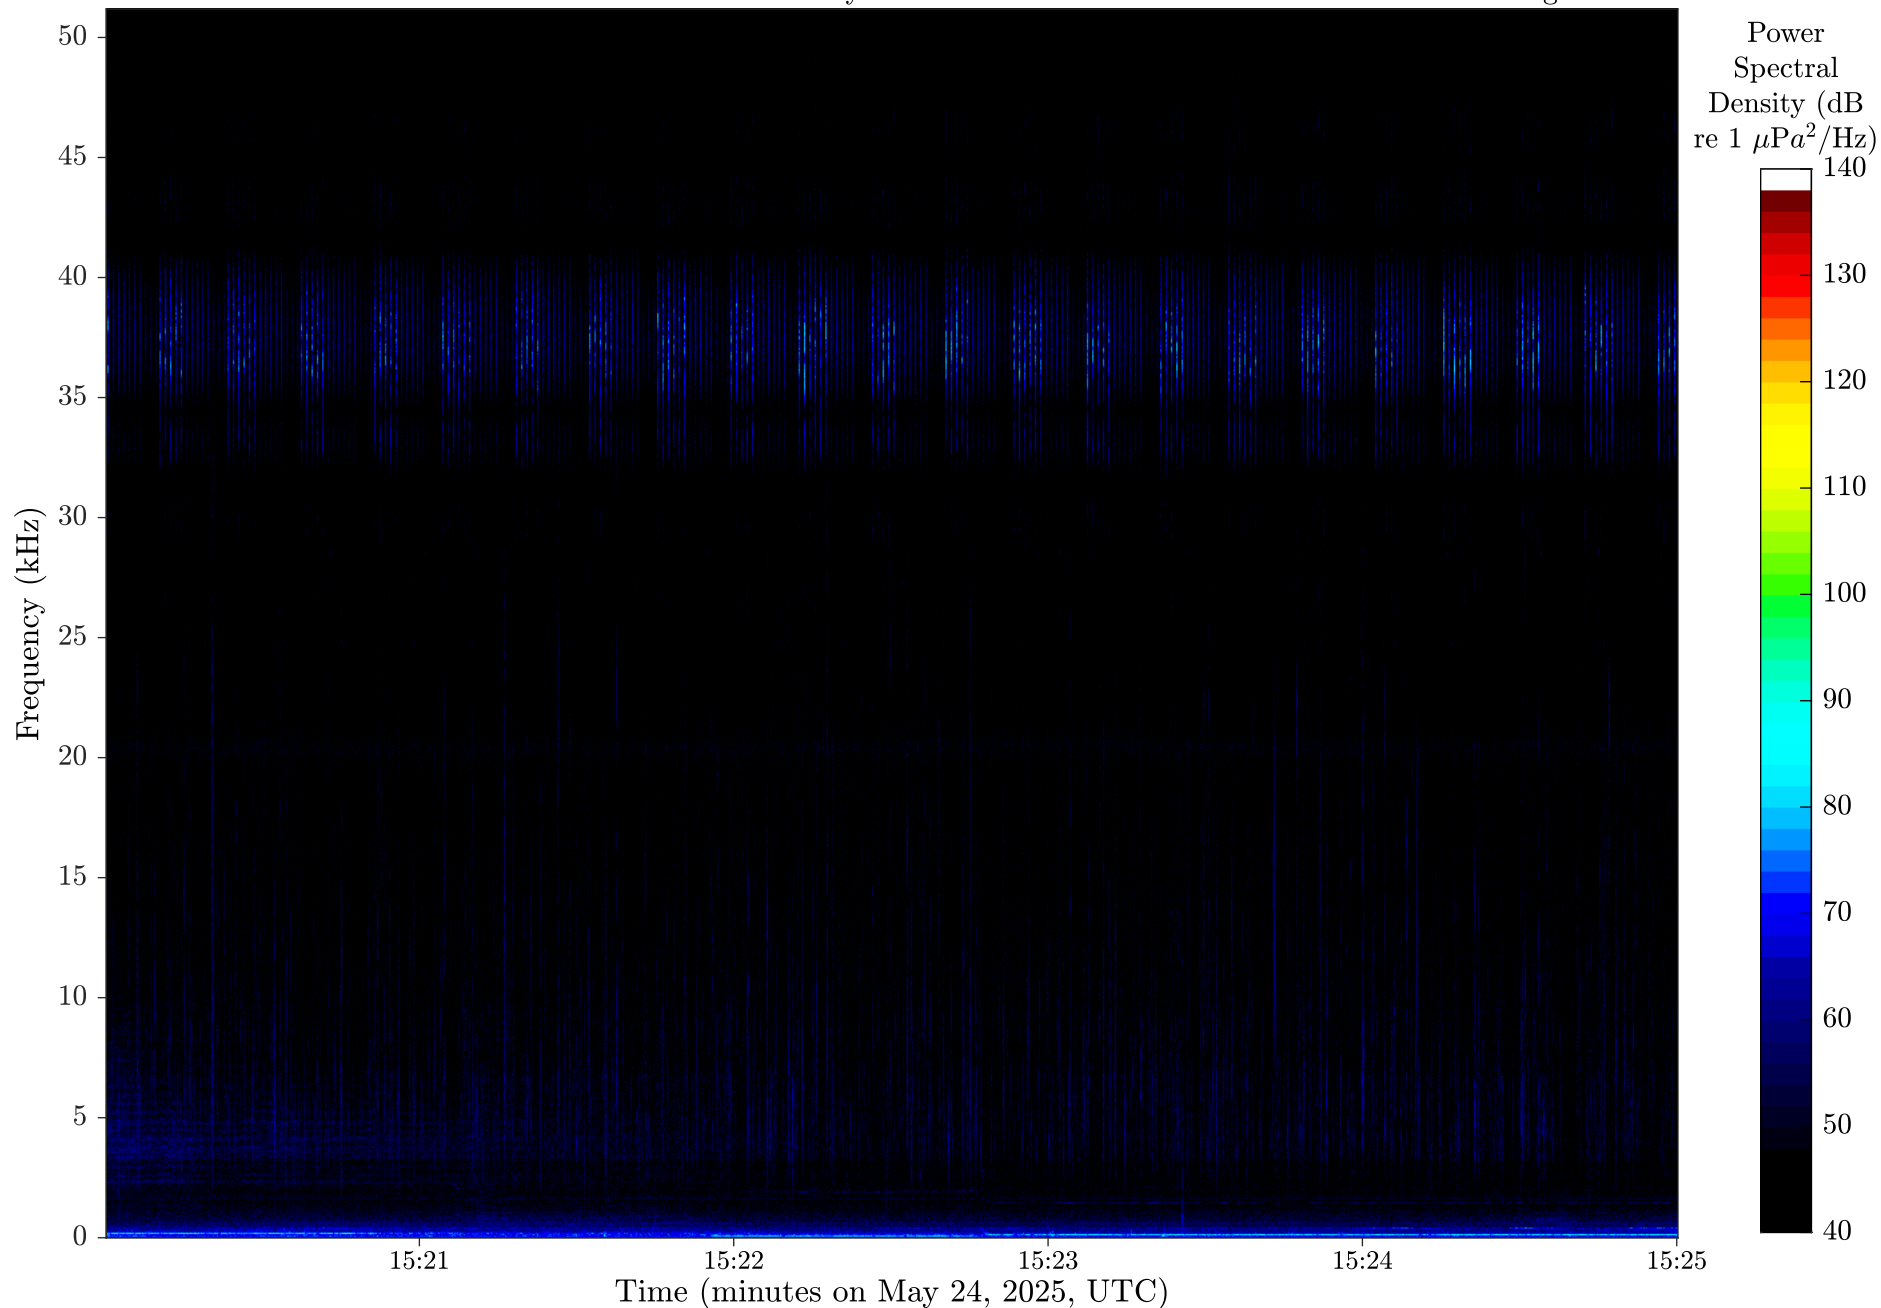


Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:32:26 UTC

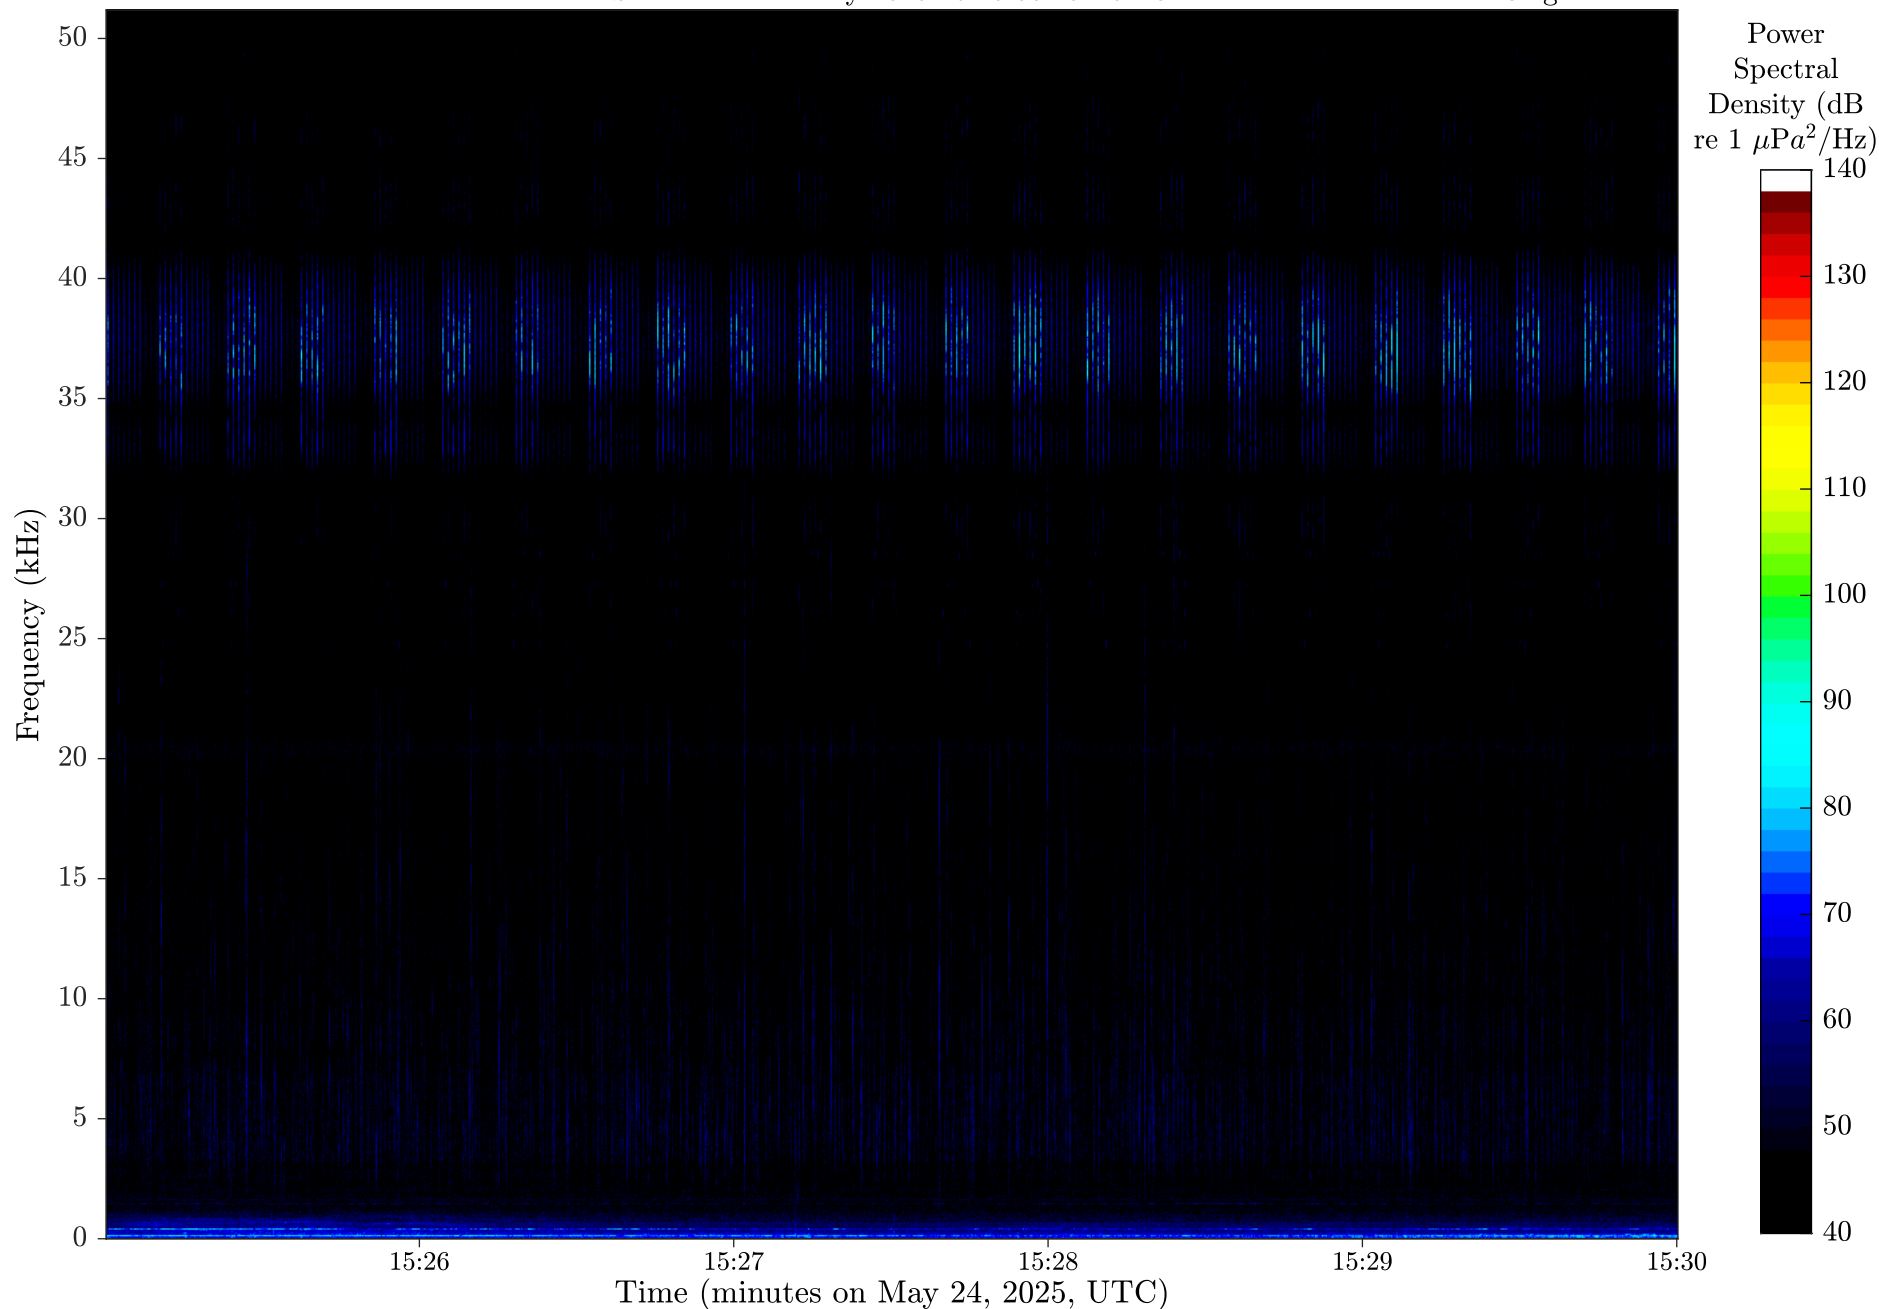

Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:32:34 UTC

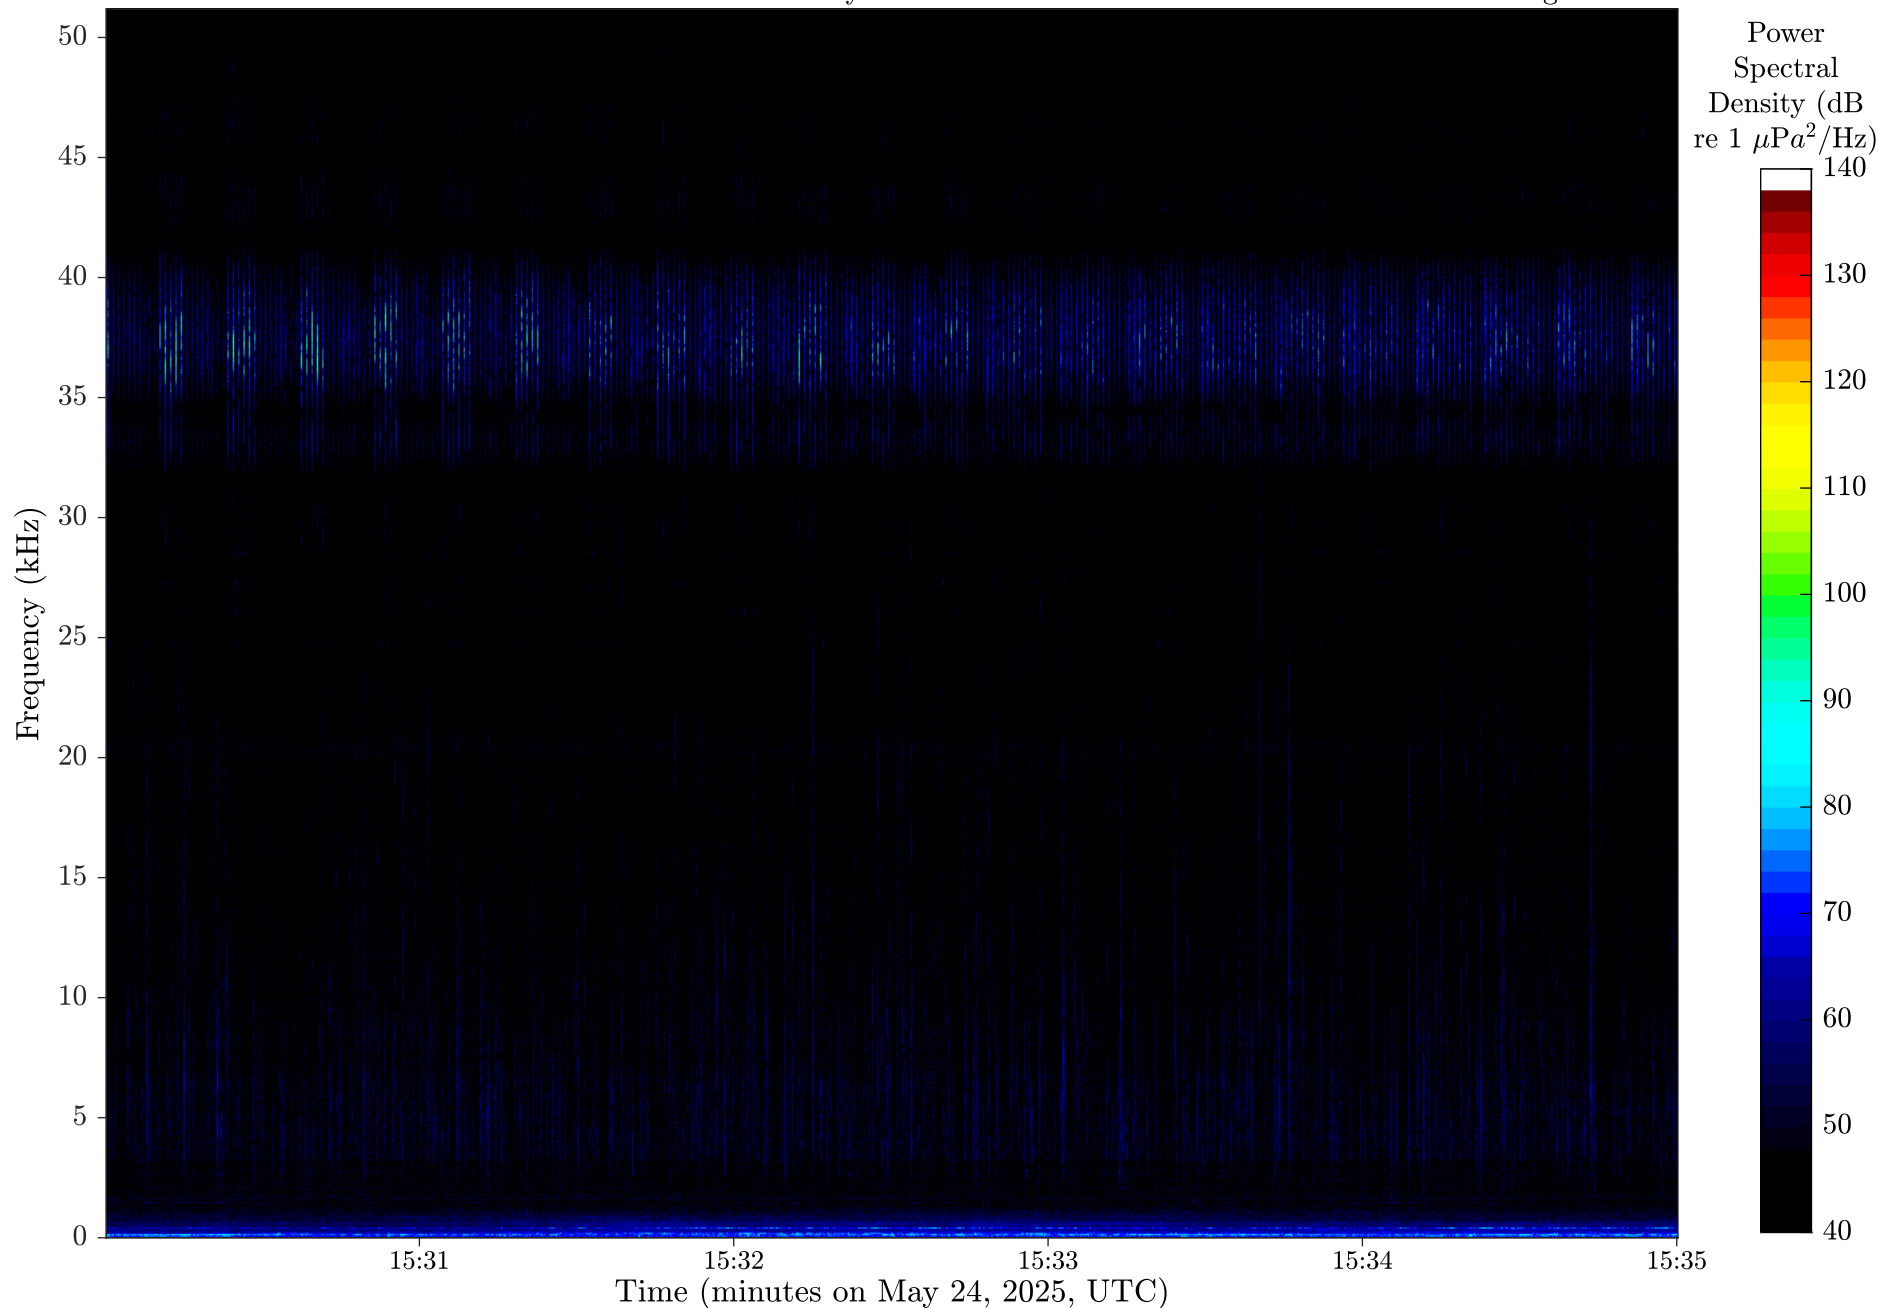

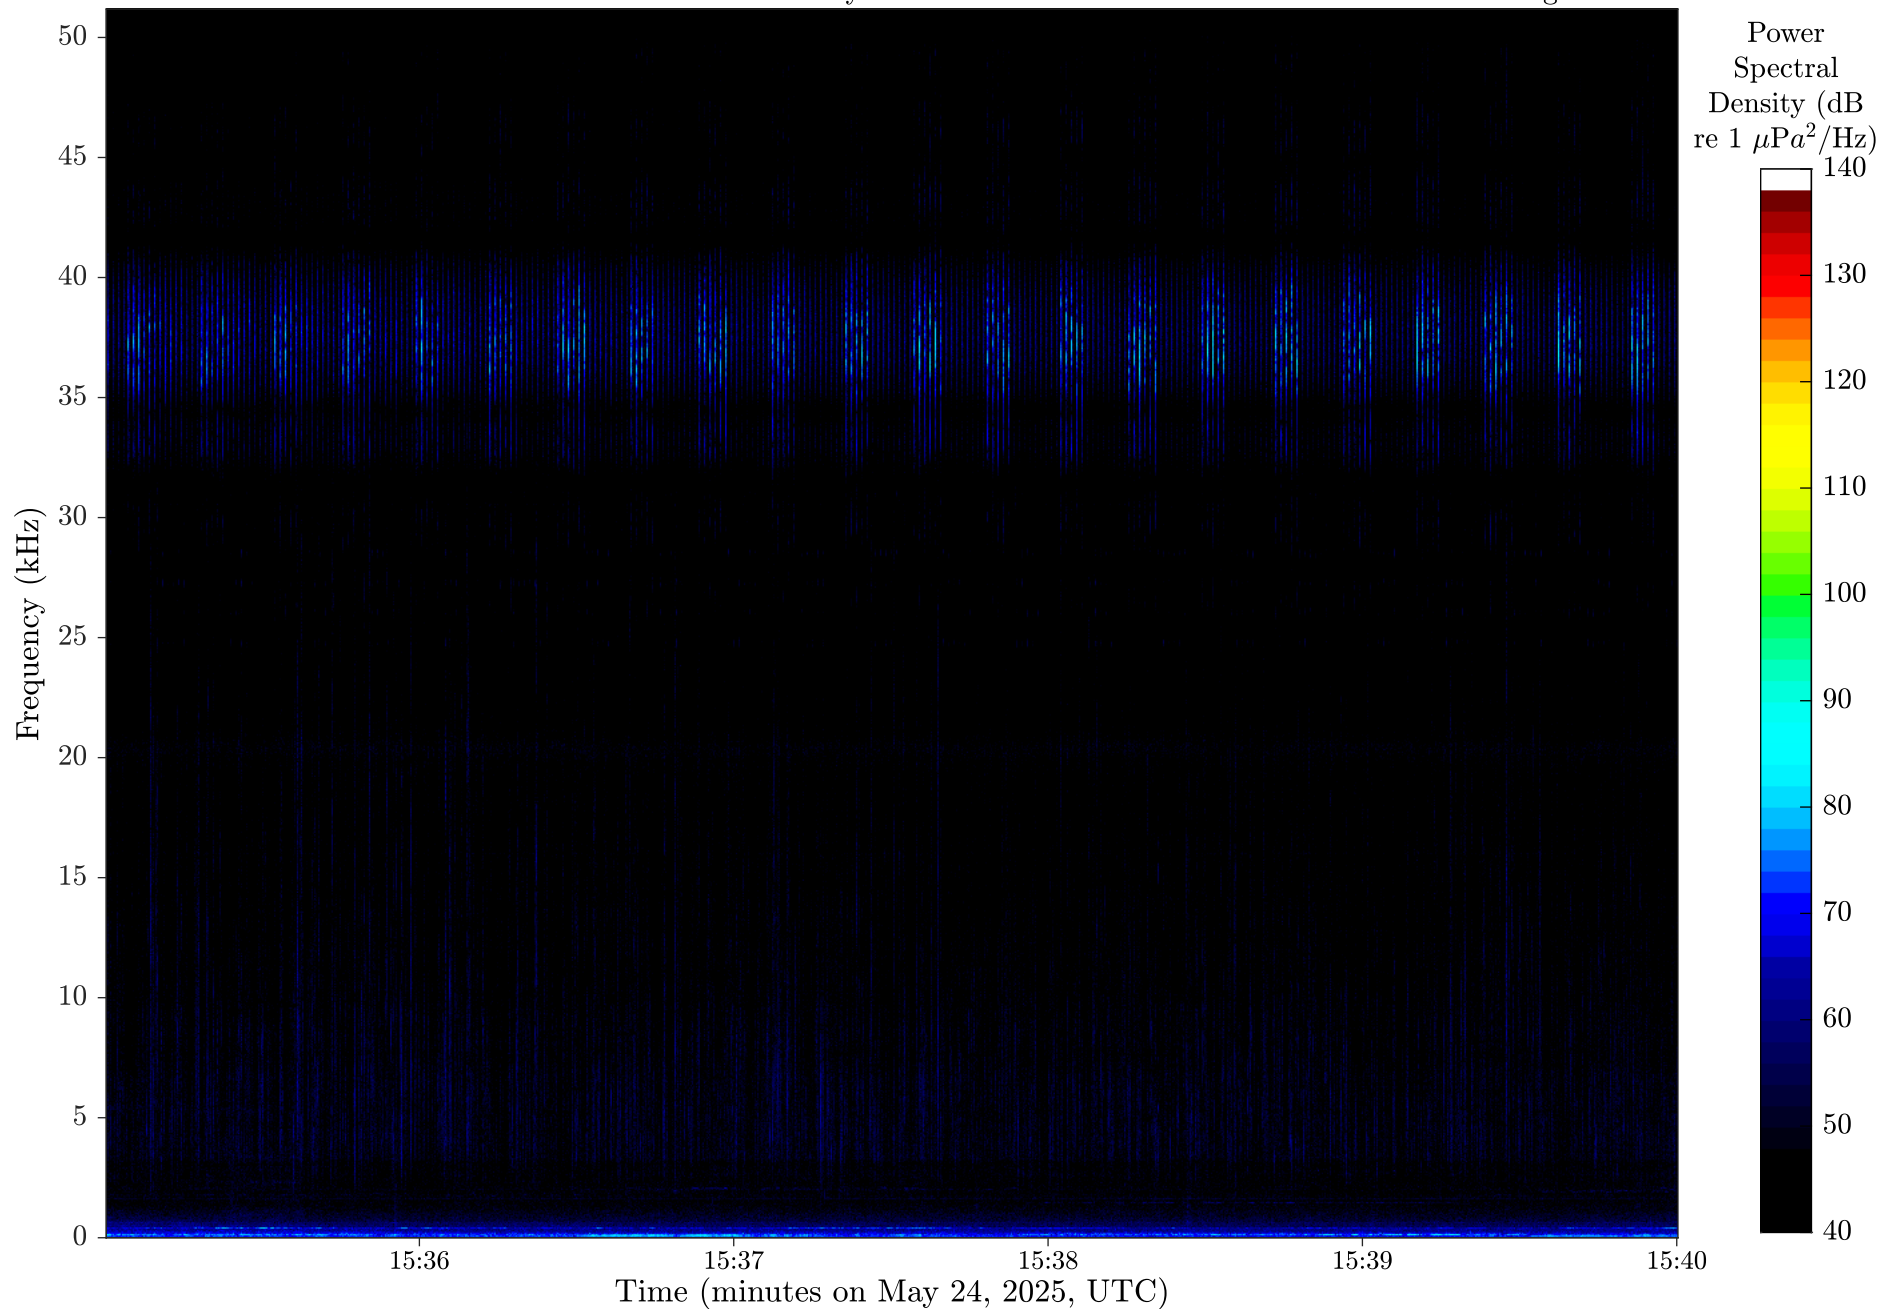


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:32:50 UTC

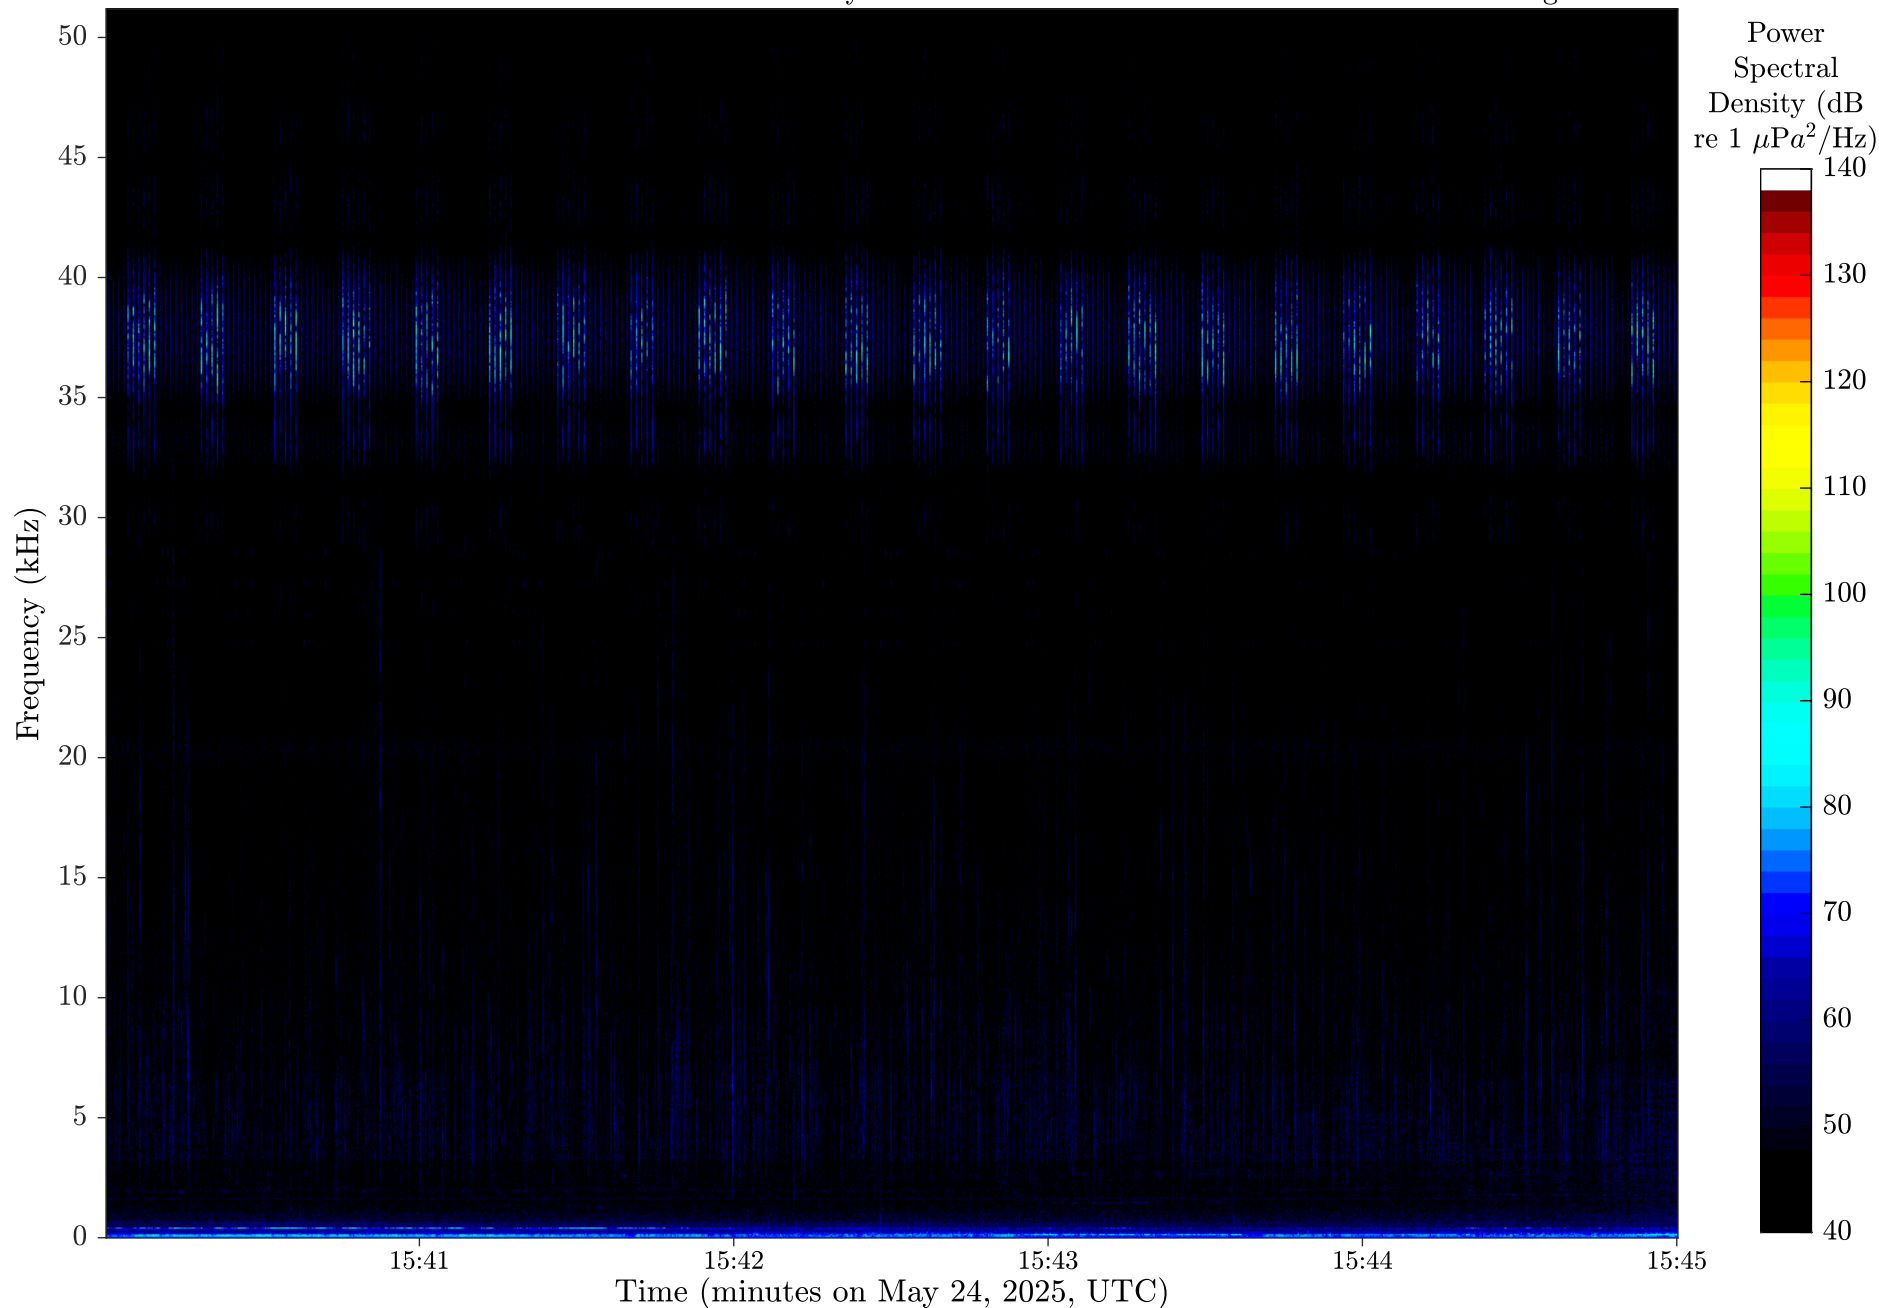

Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:32:59 UTC

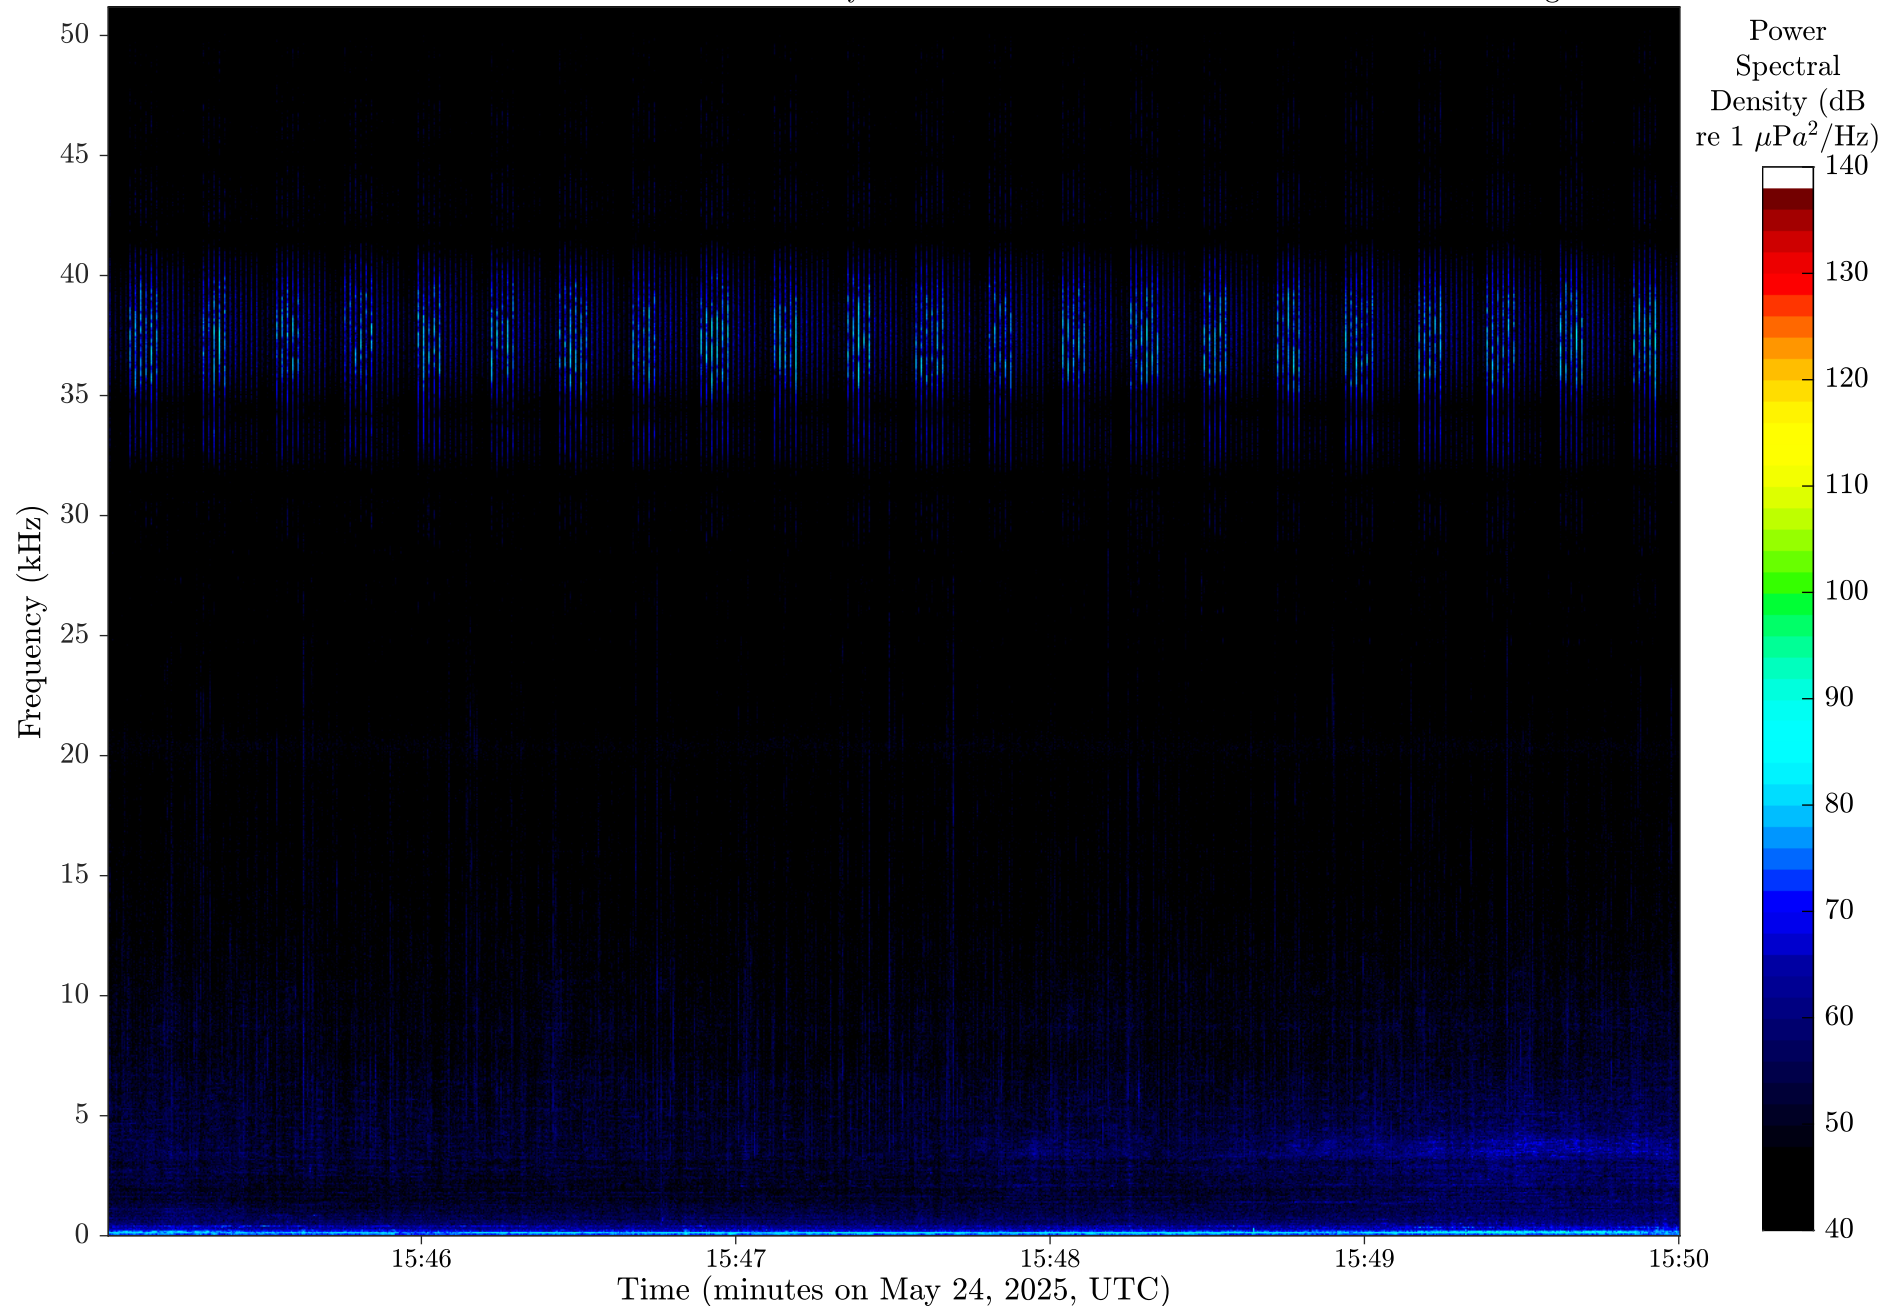

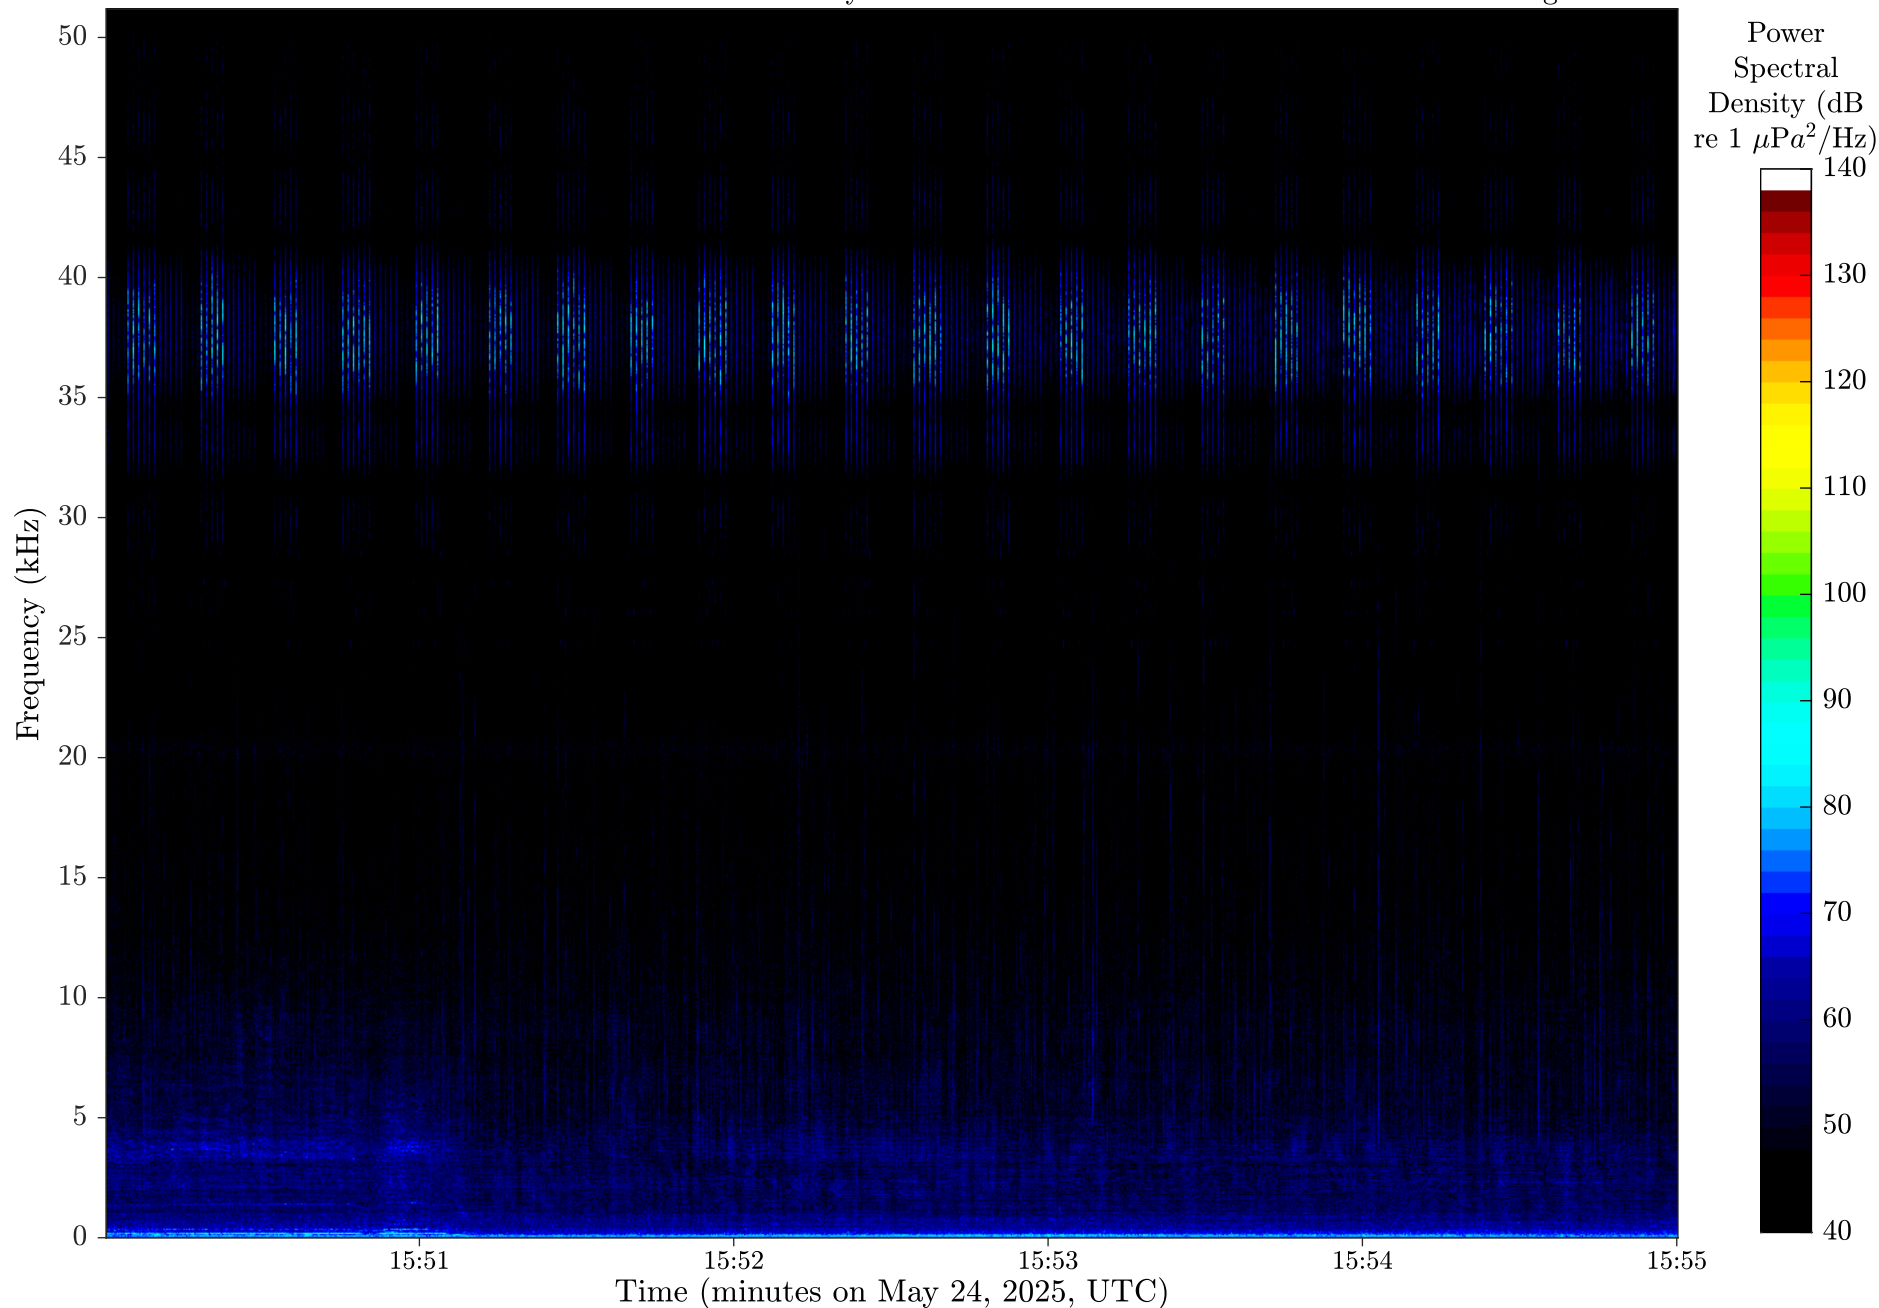


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:33:15 UTC

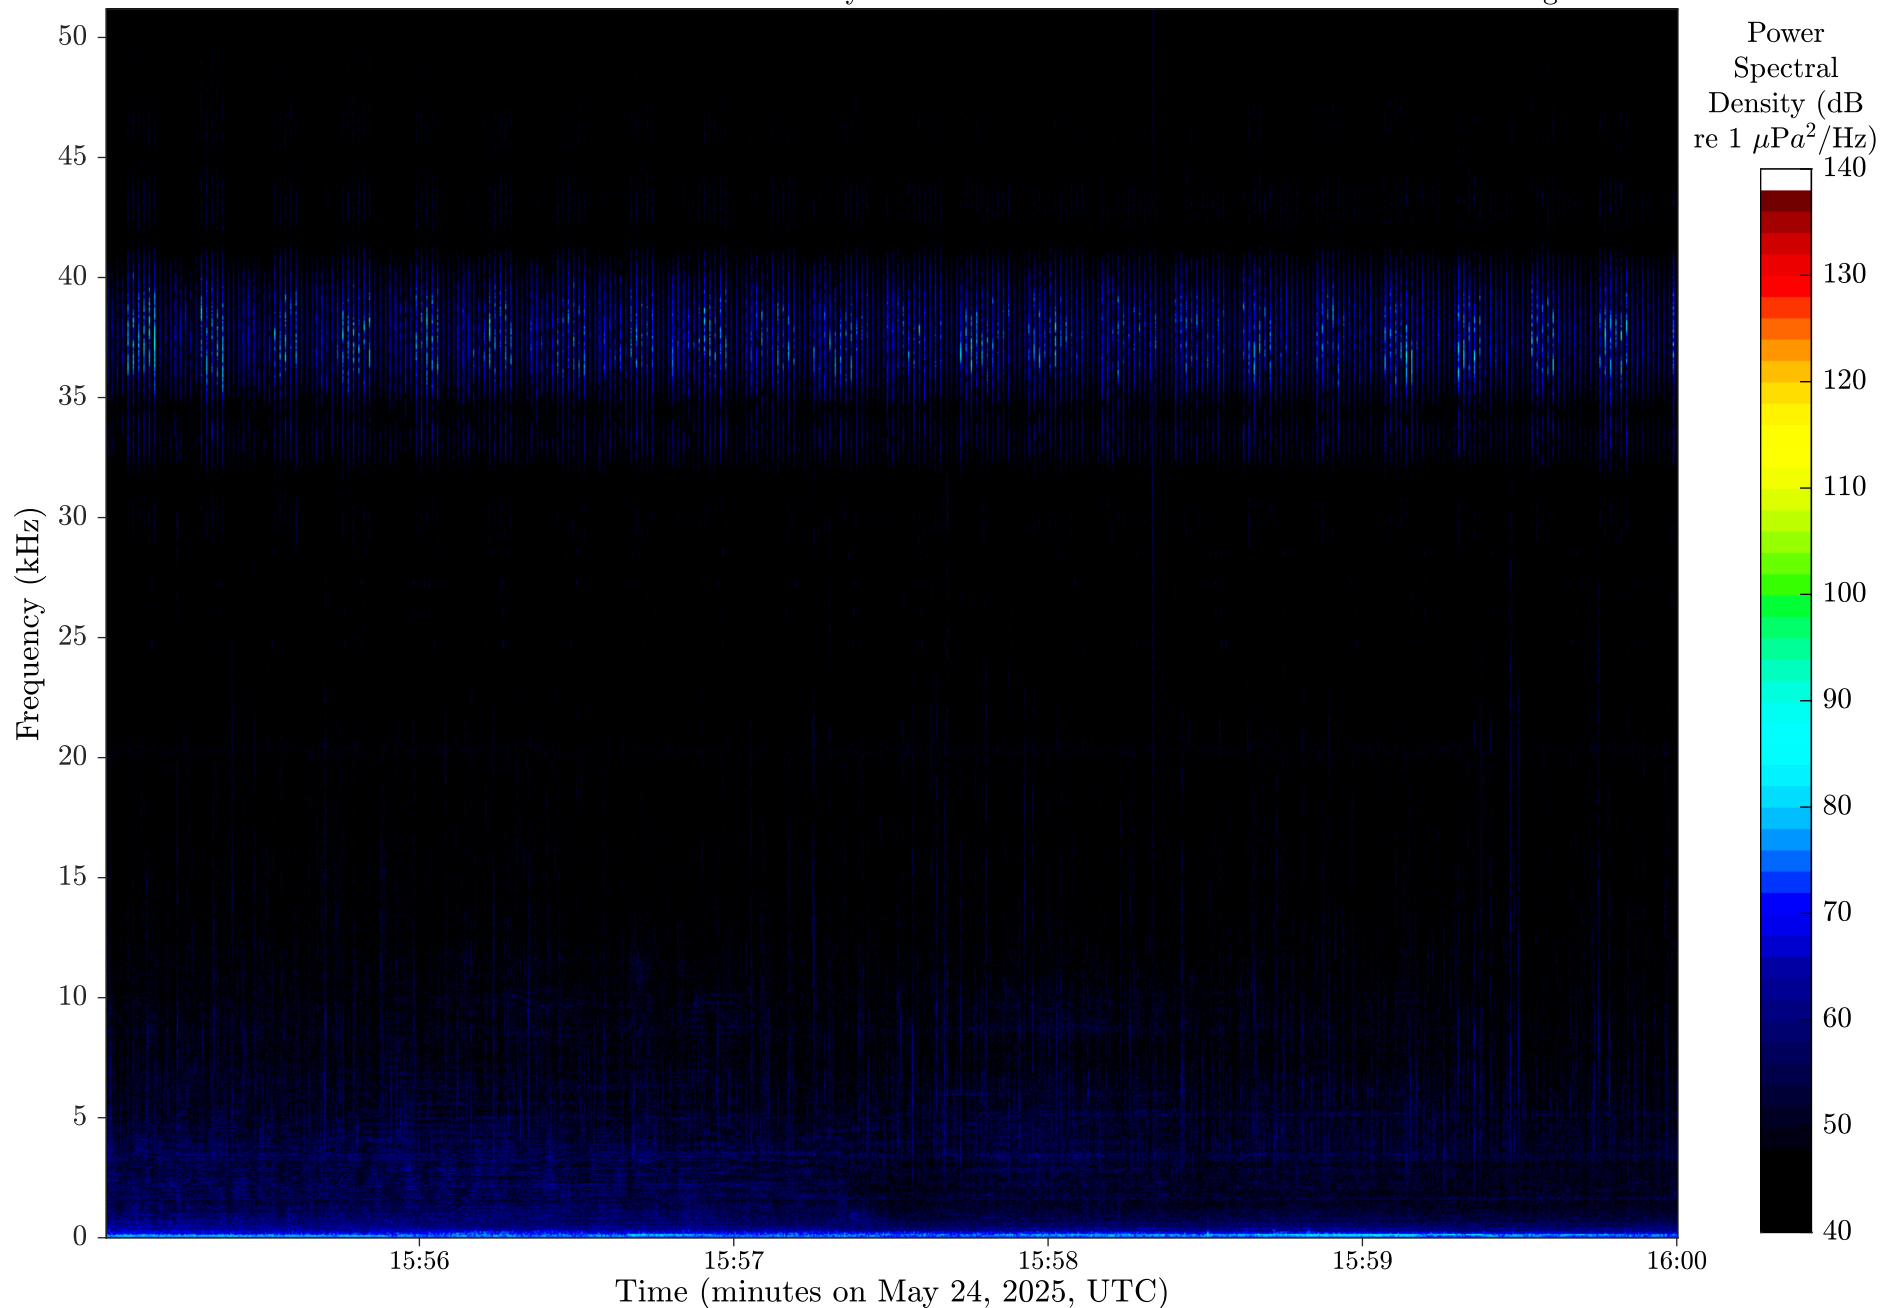


Comments: 31 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:33:24 UTC

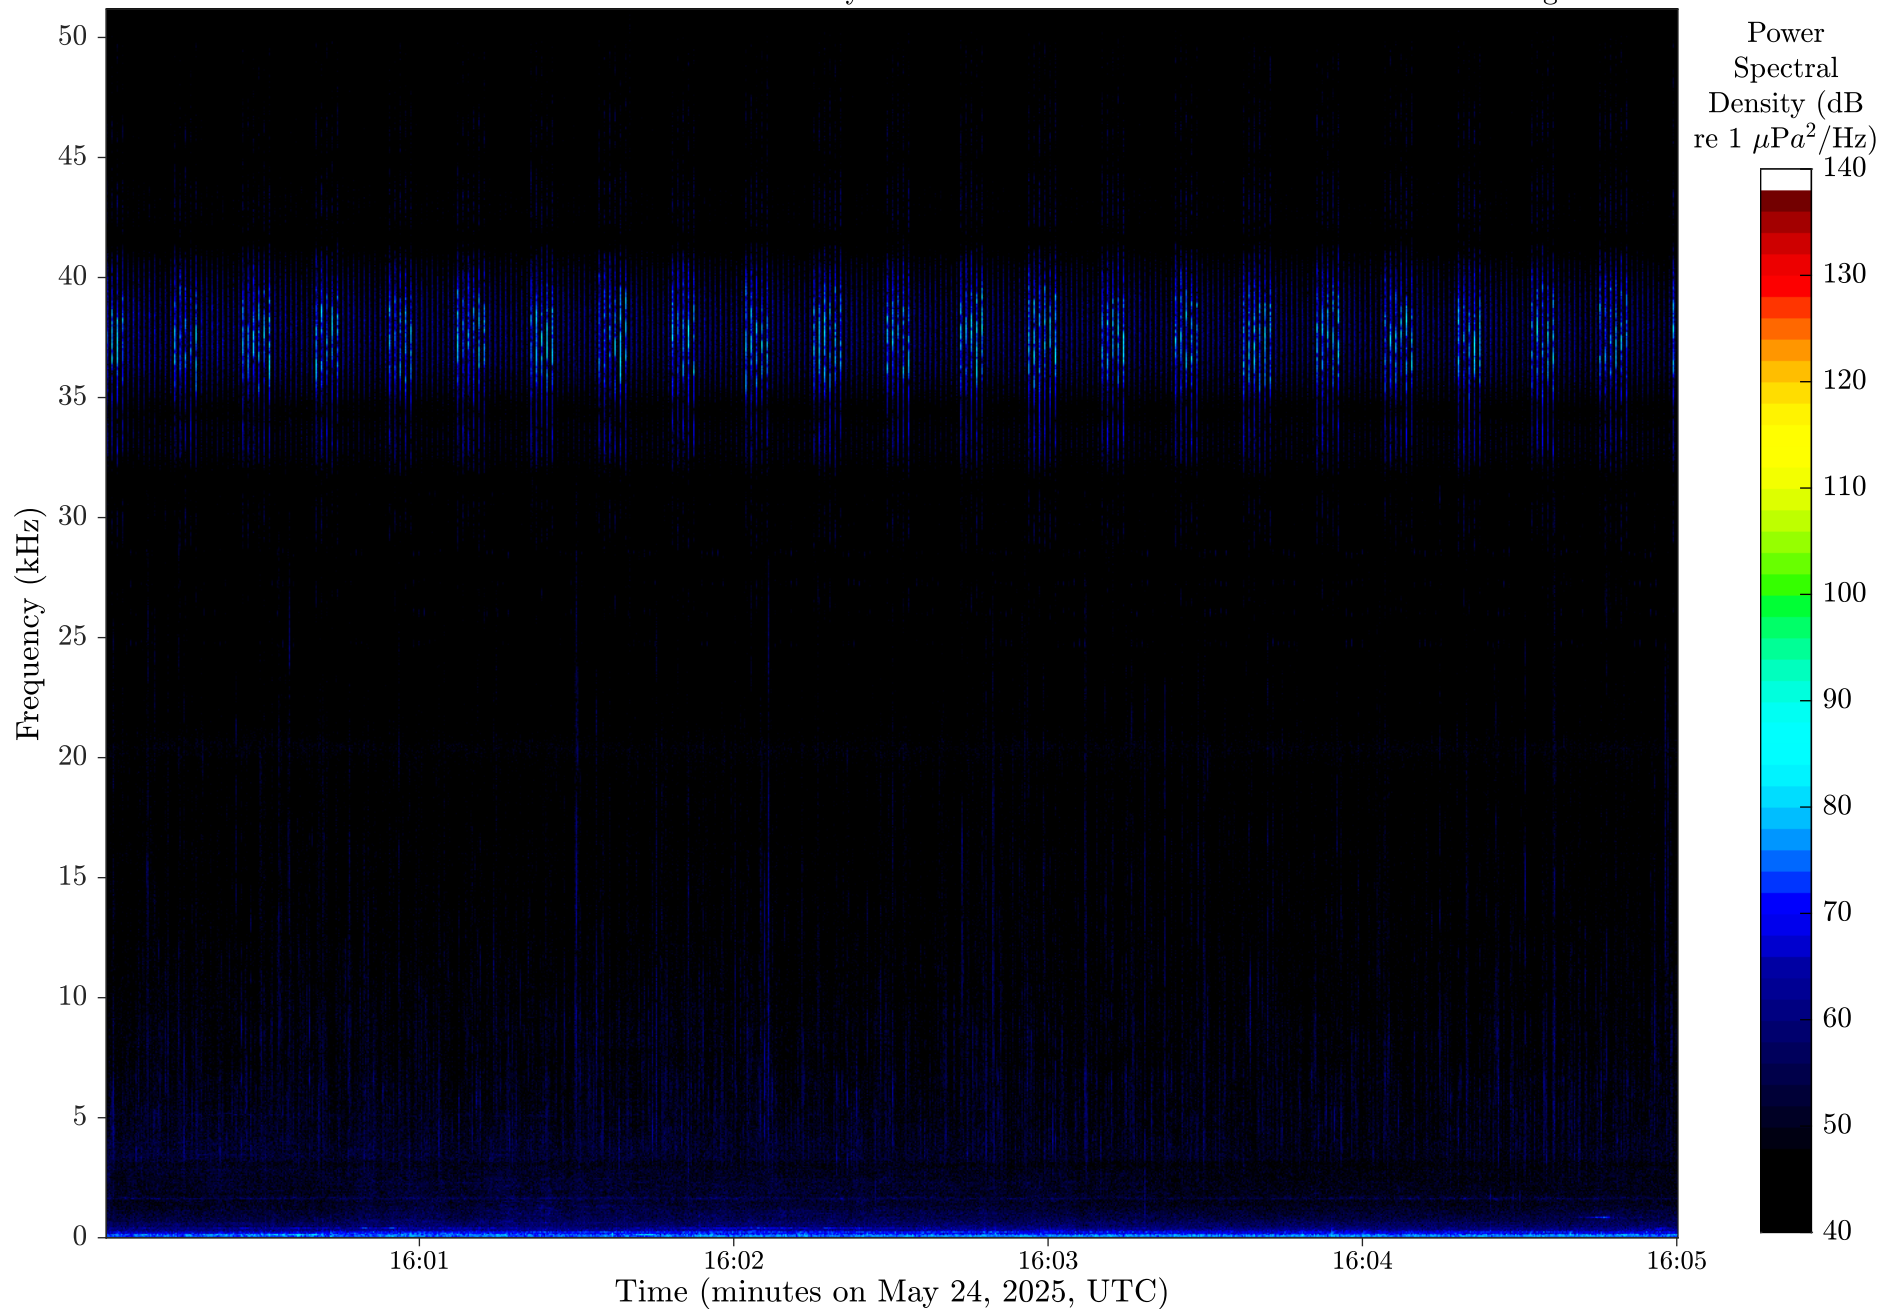


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:33:32 UTC

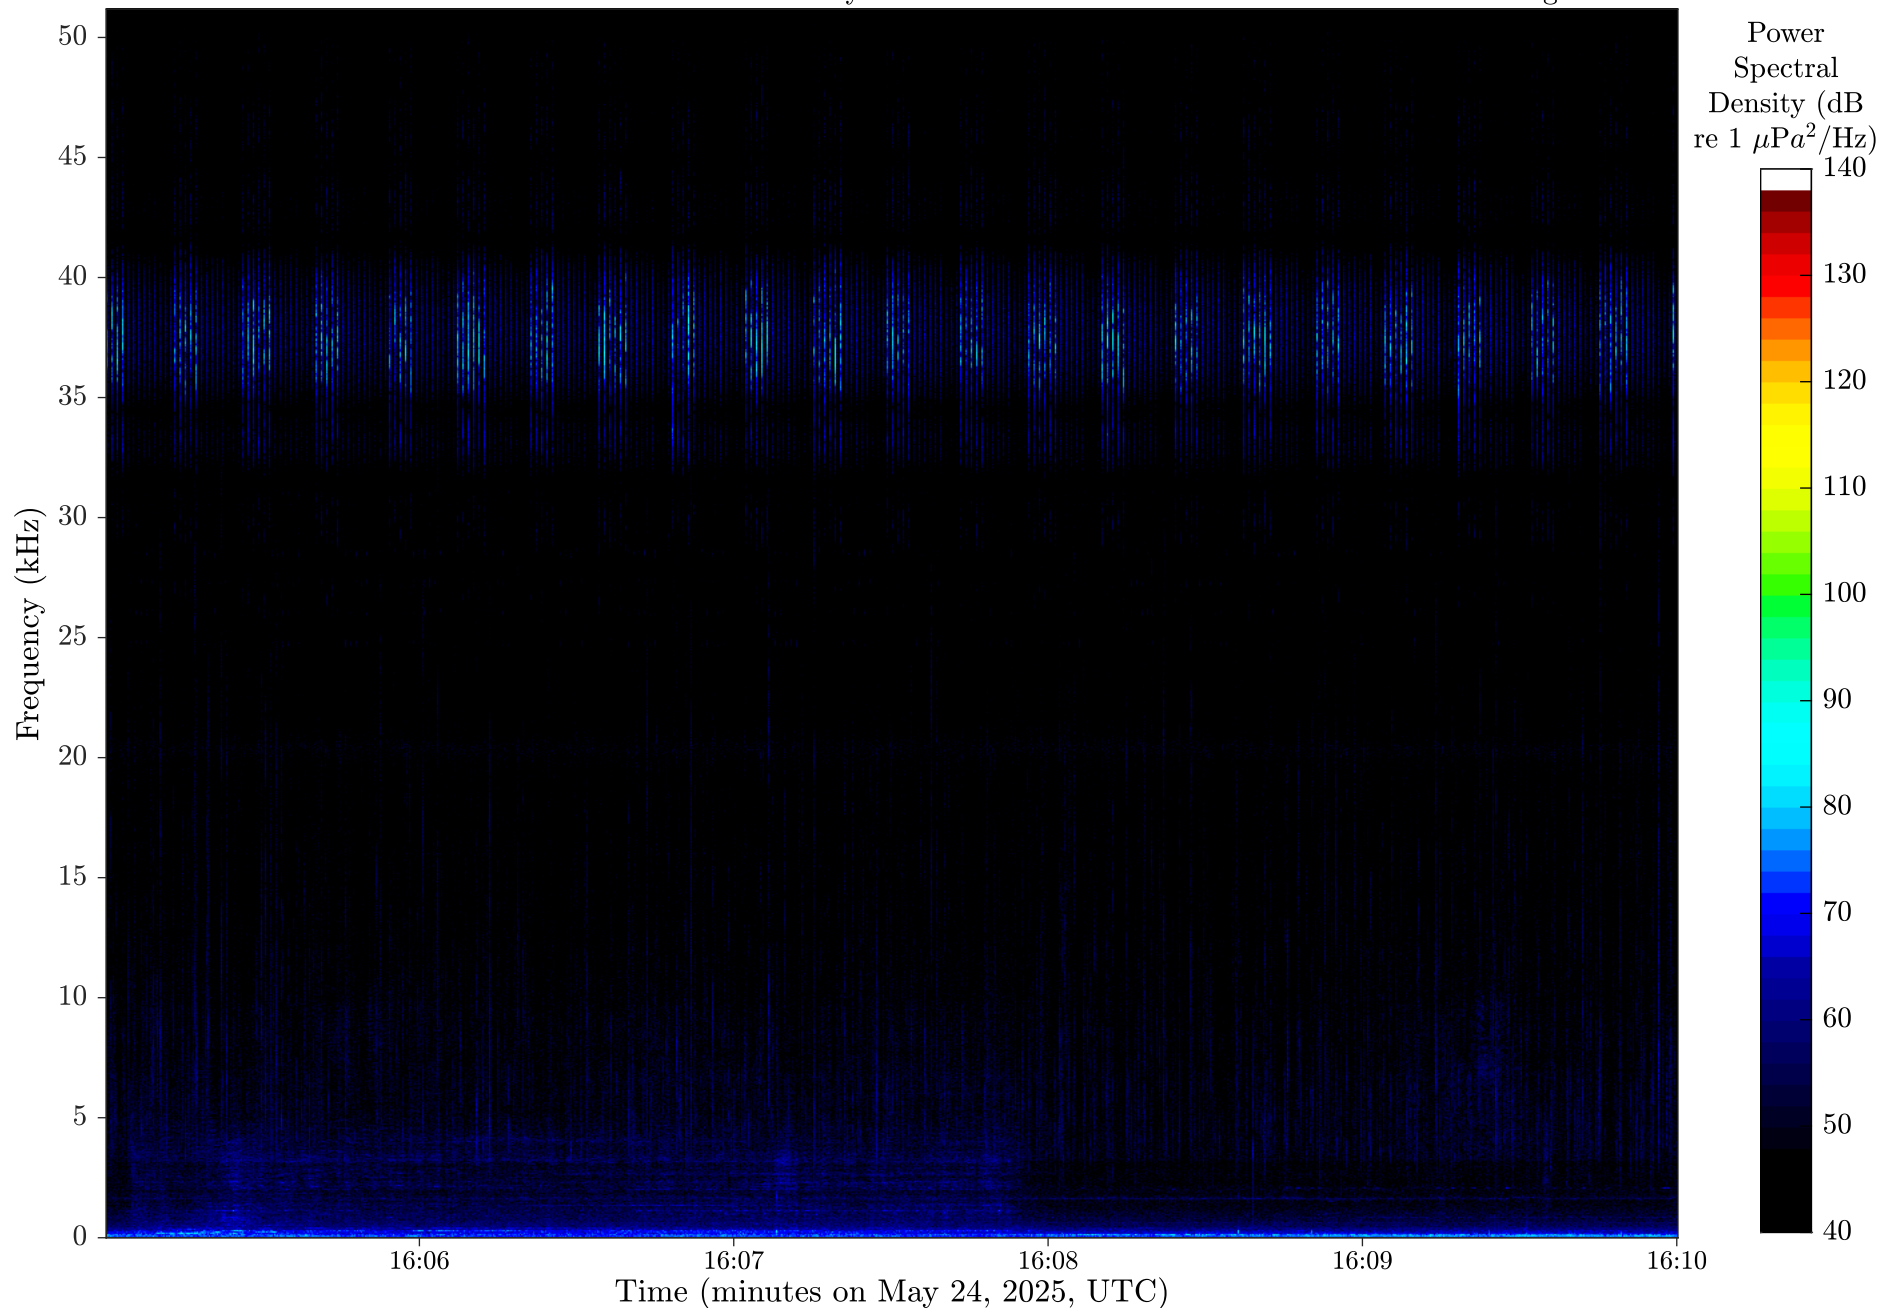


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:33:40 UTC

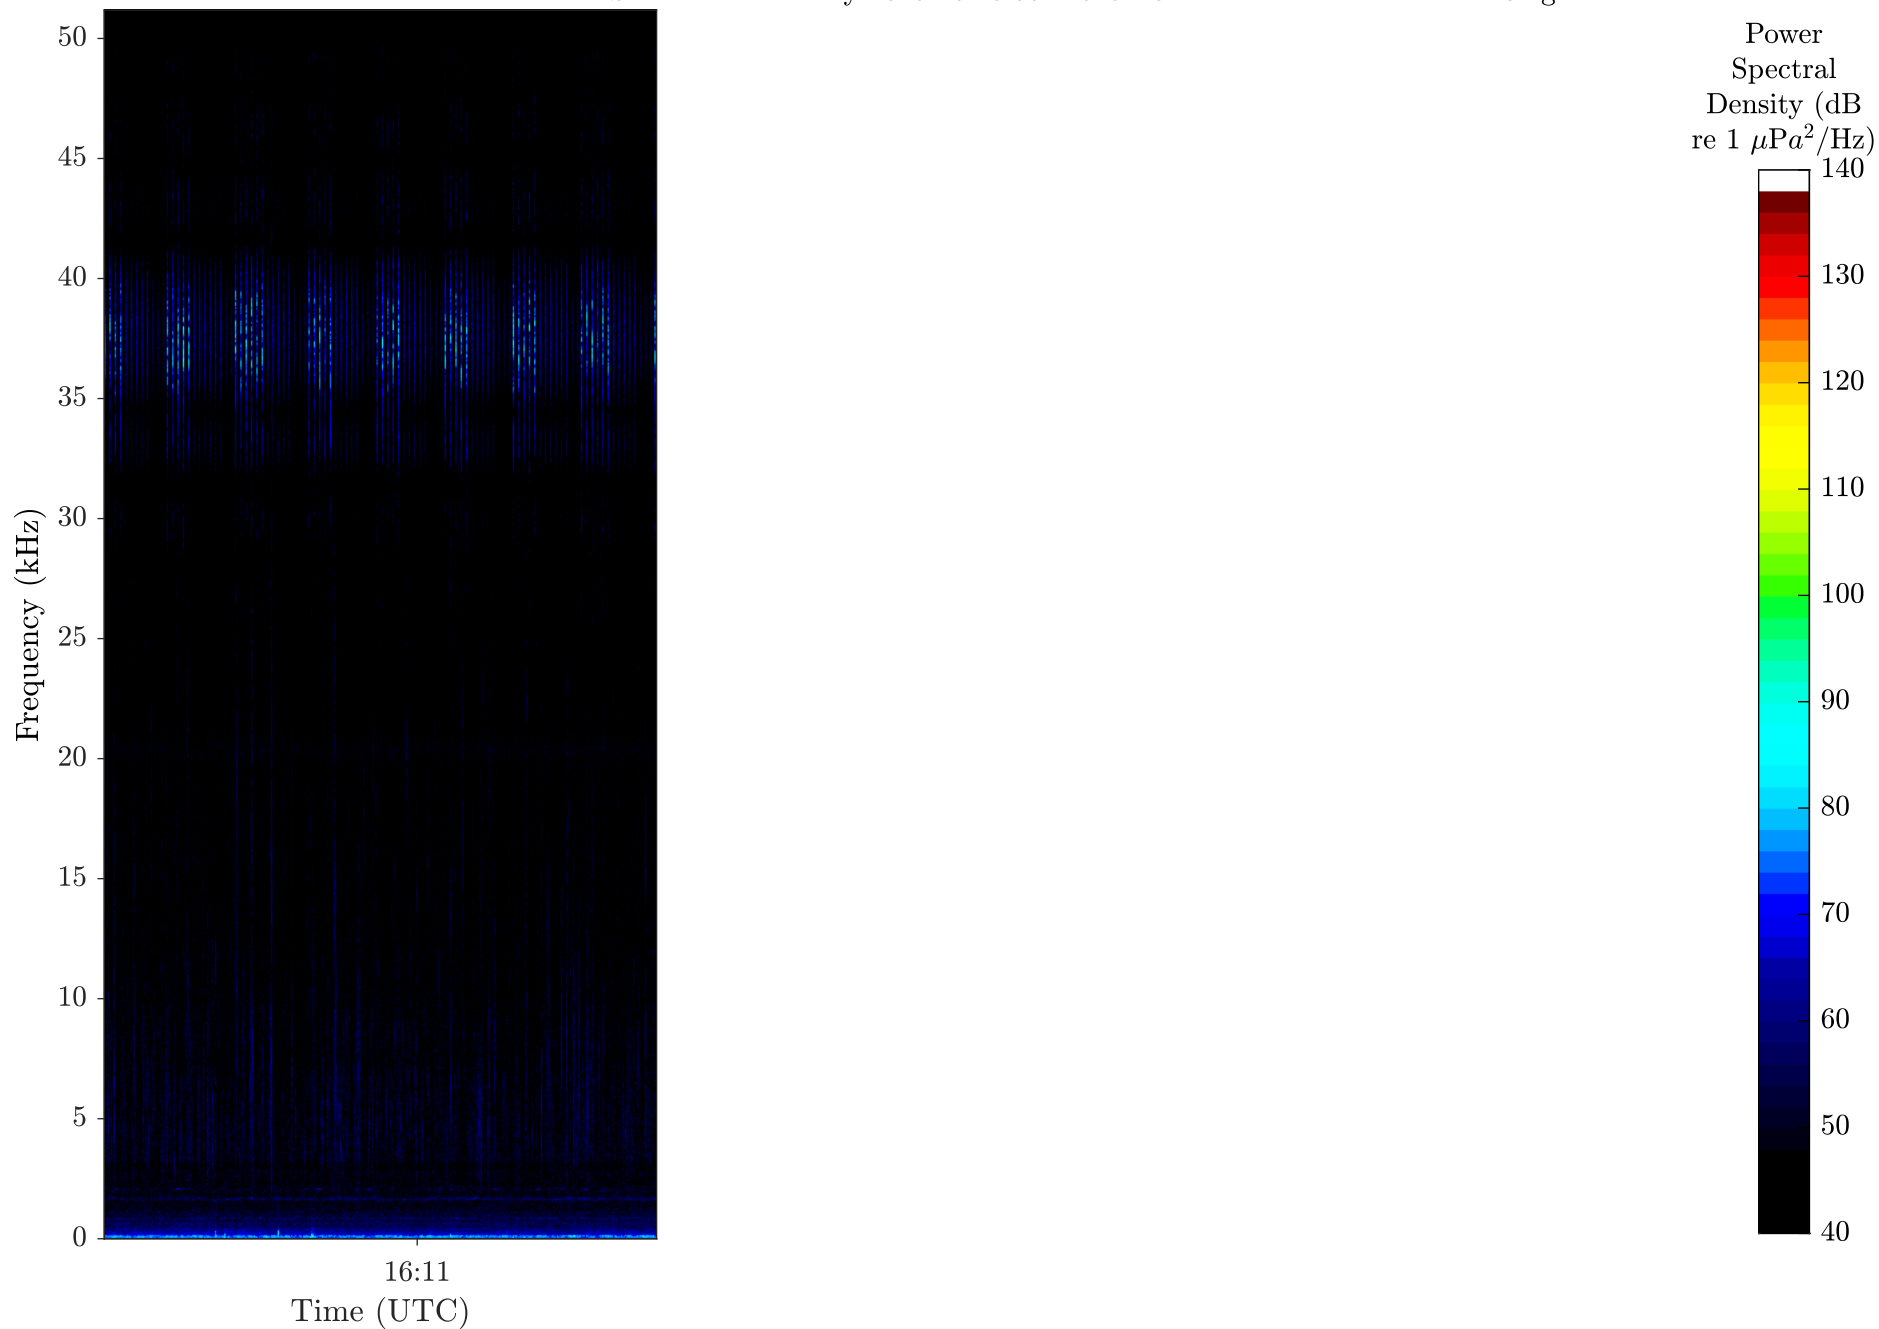

Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:33:45 UTC

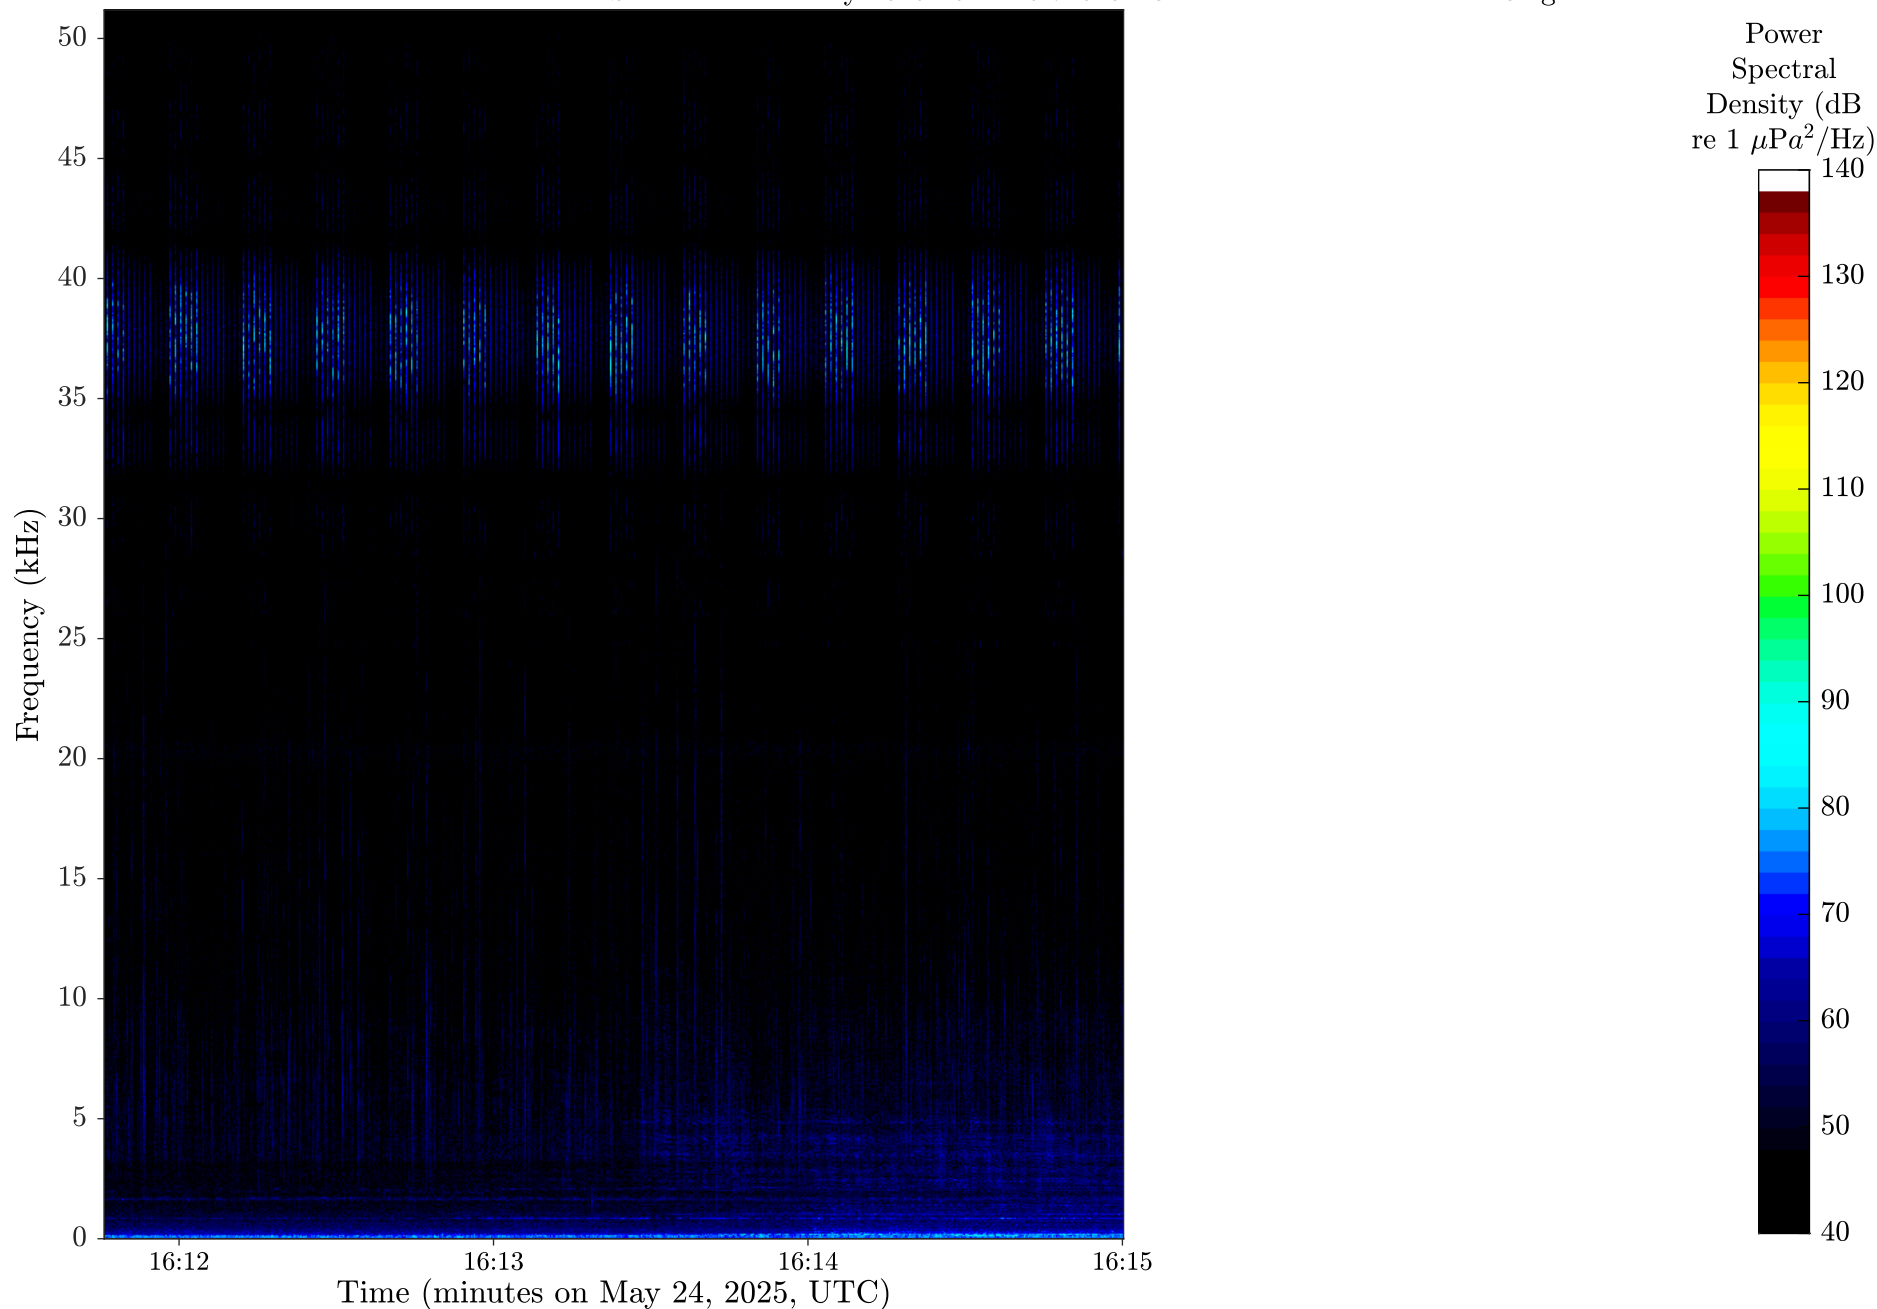


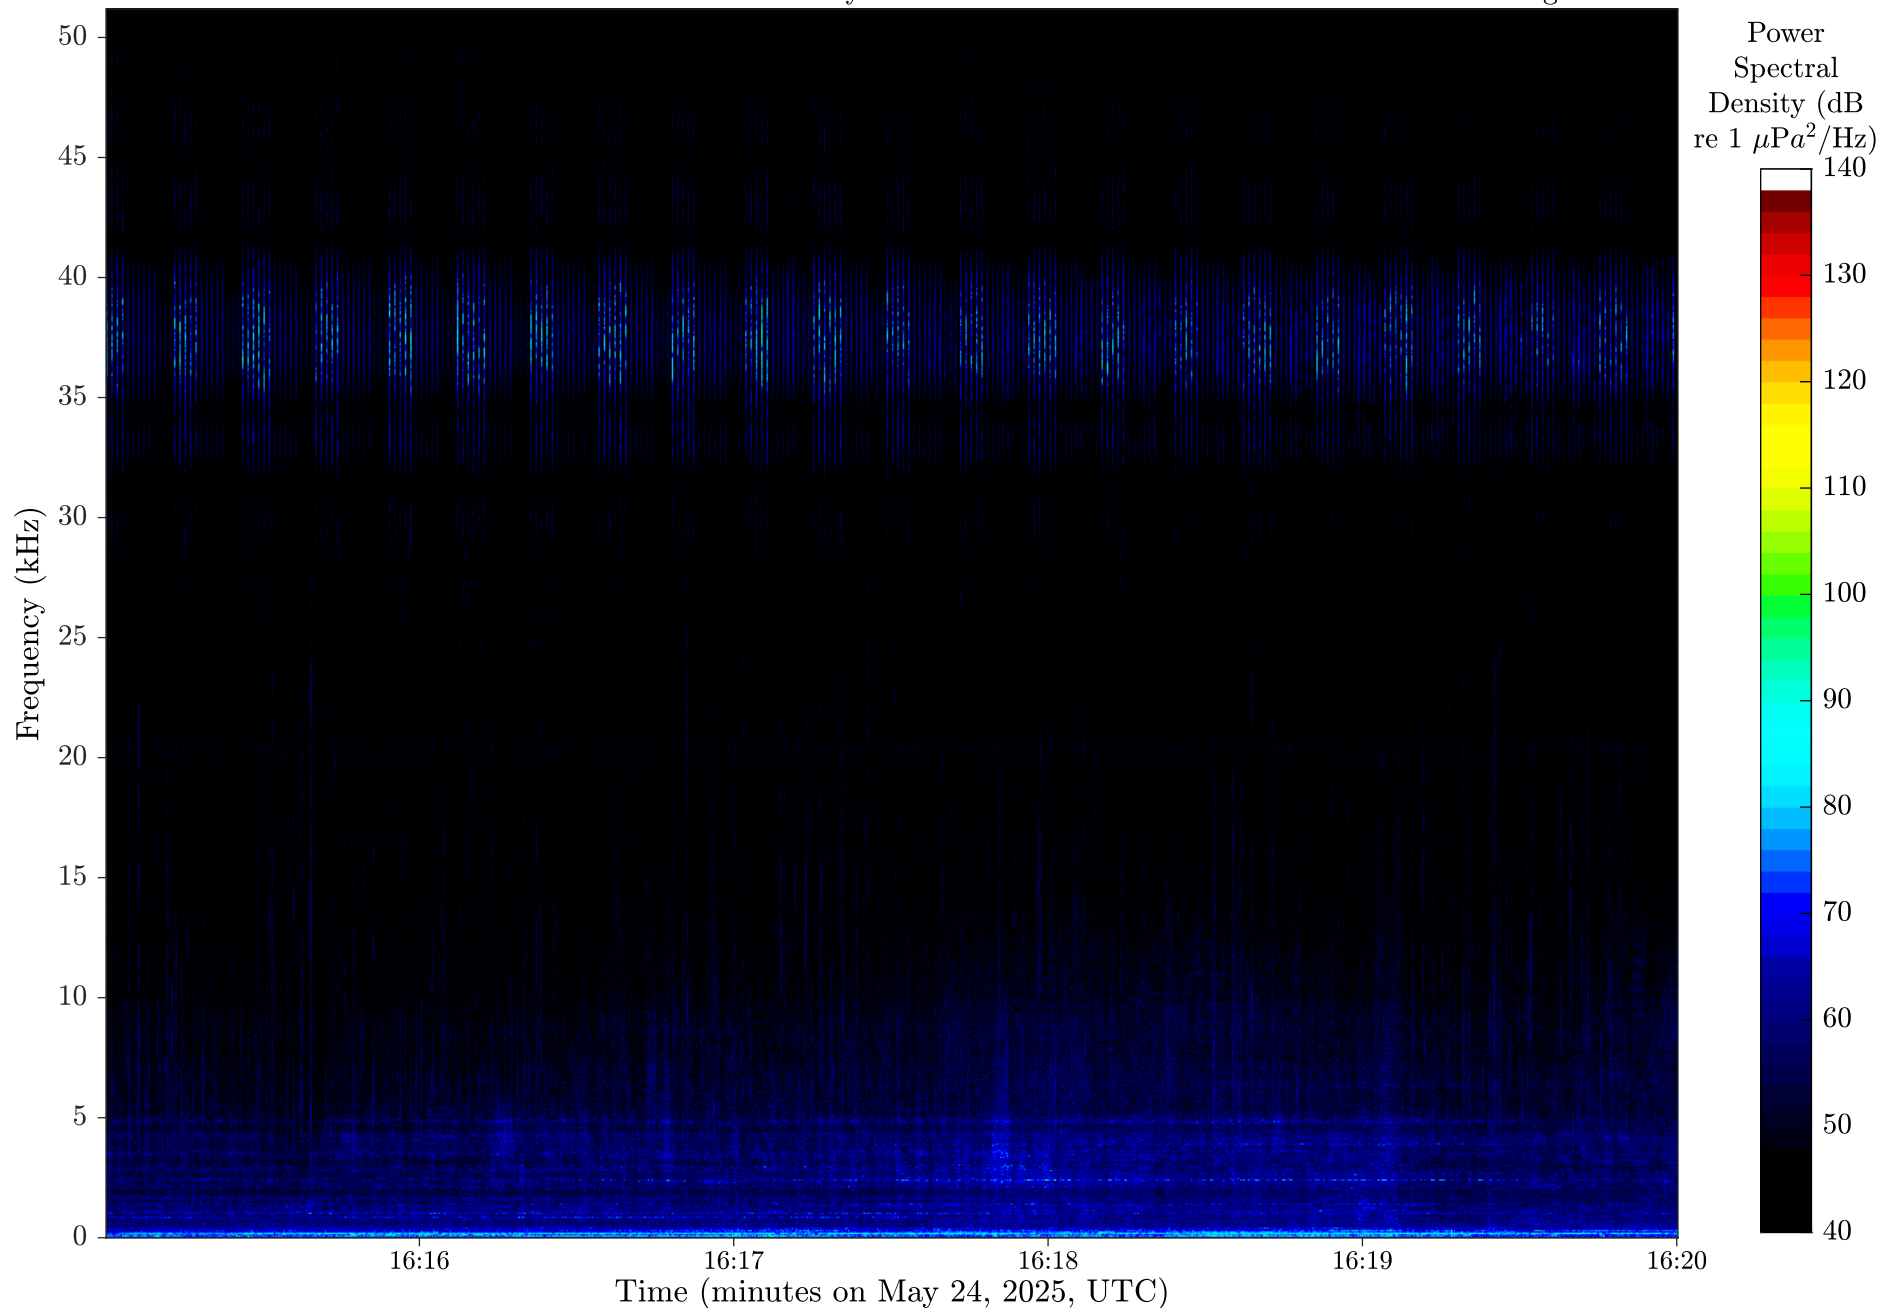

Comments: 29.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:33:58 UTC

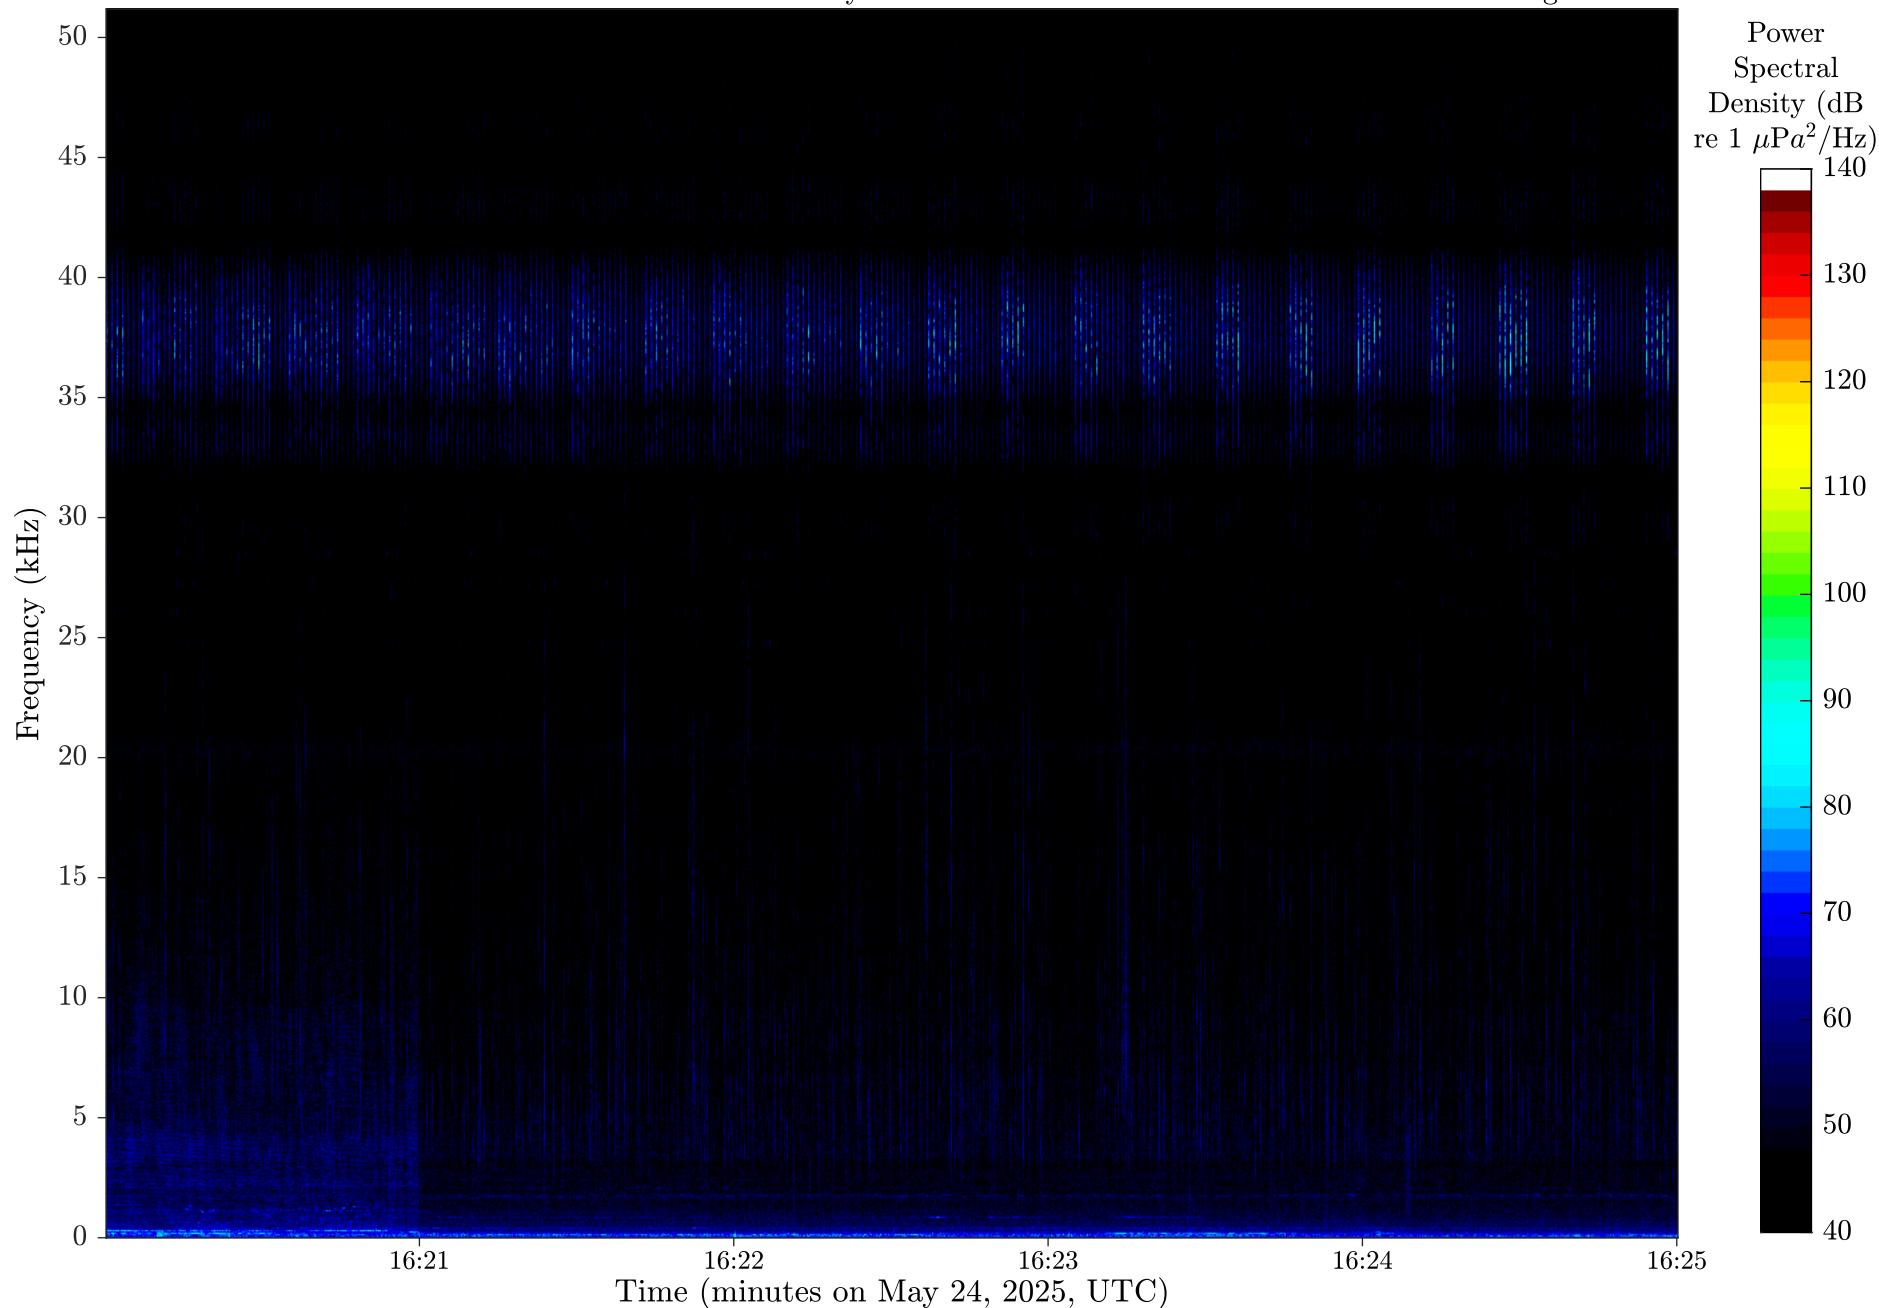

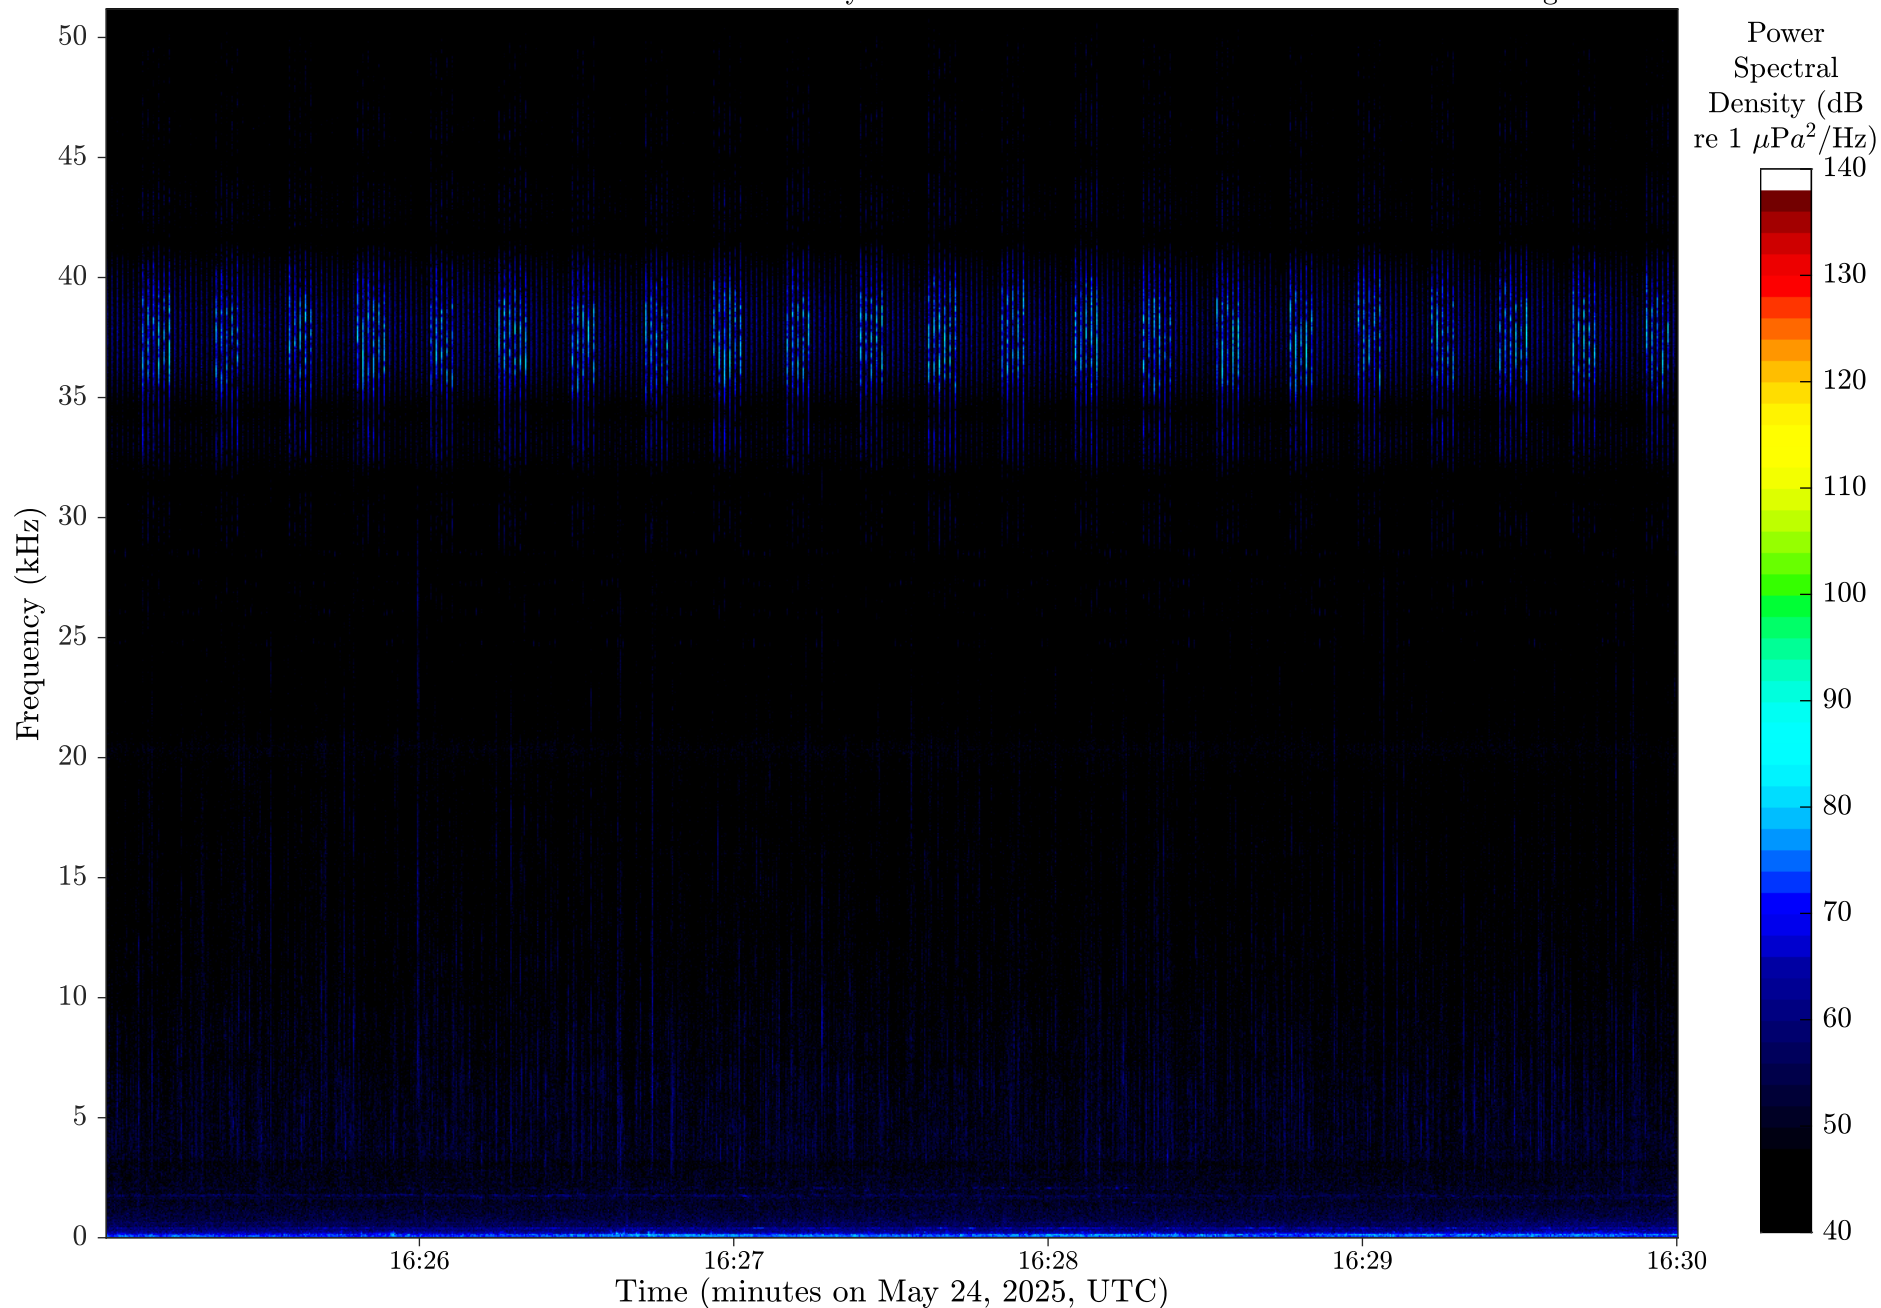


Comments: 29.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:14 UTC

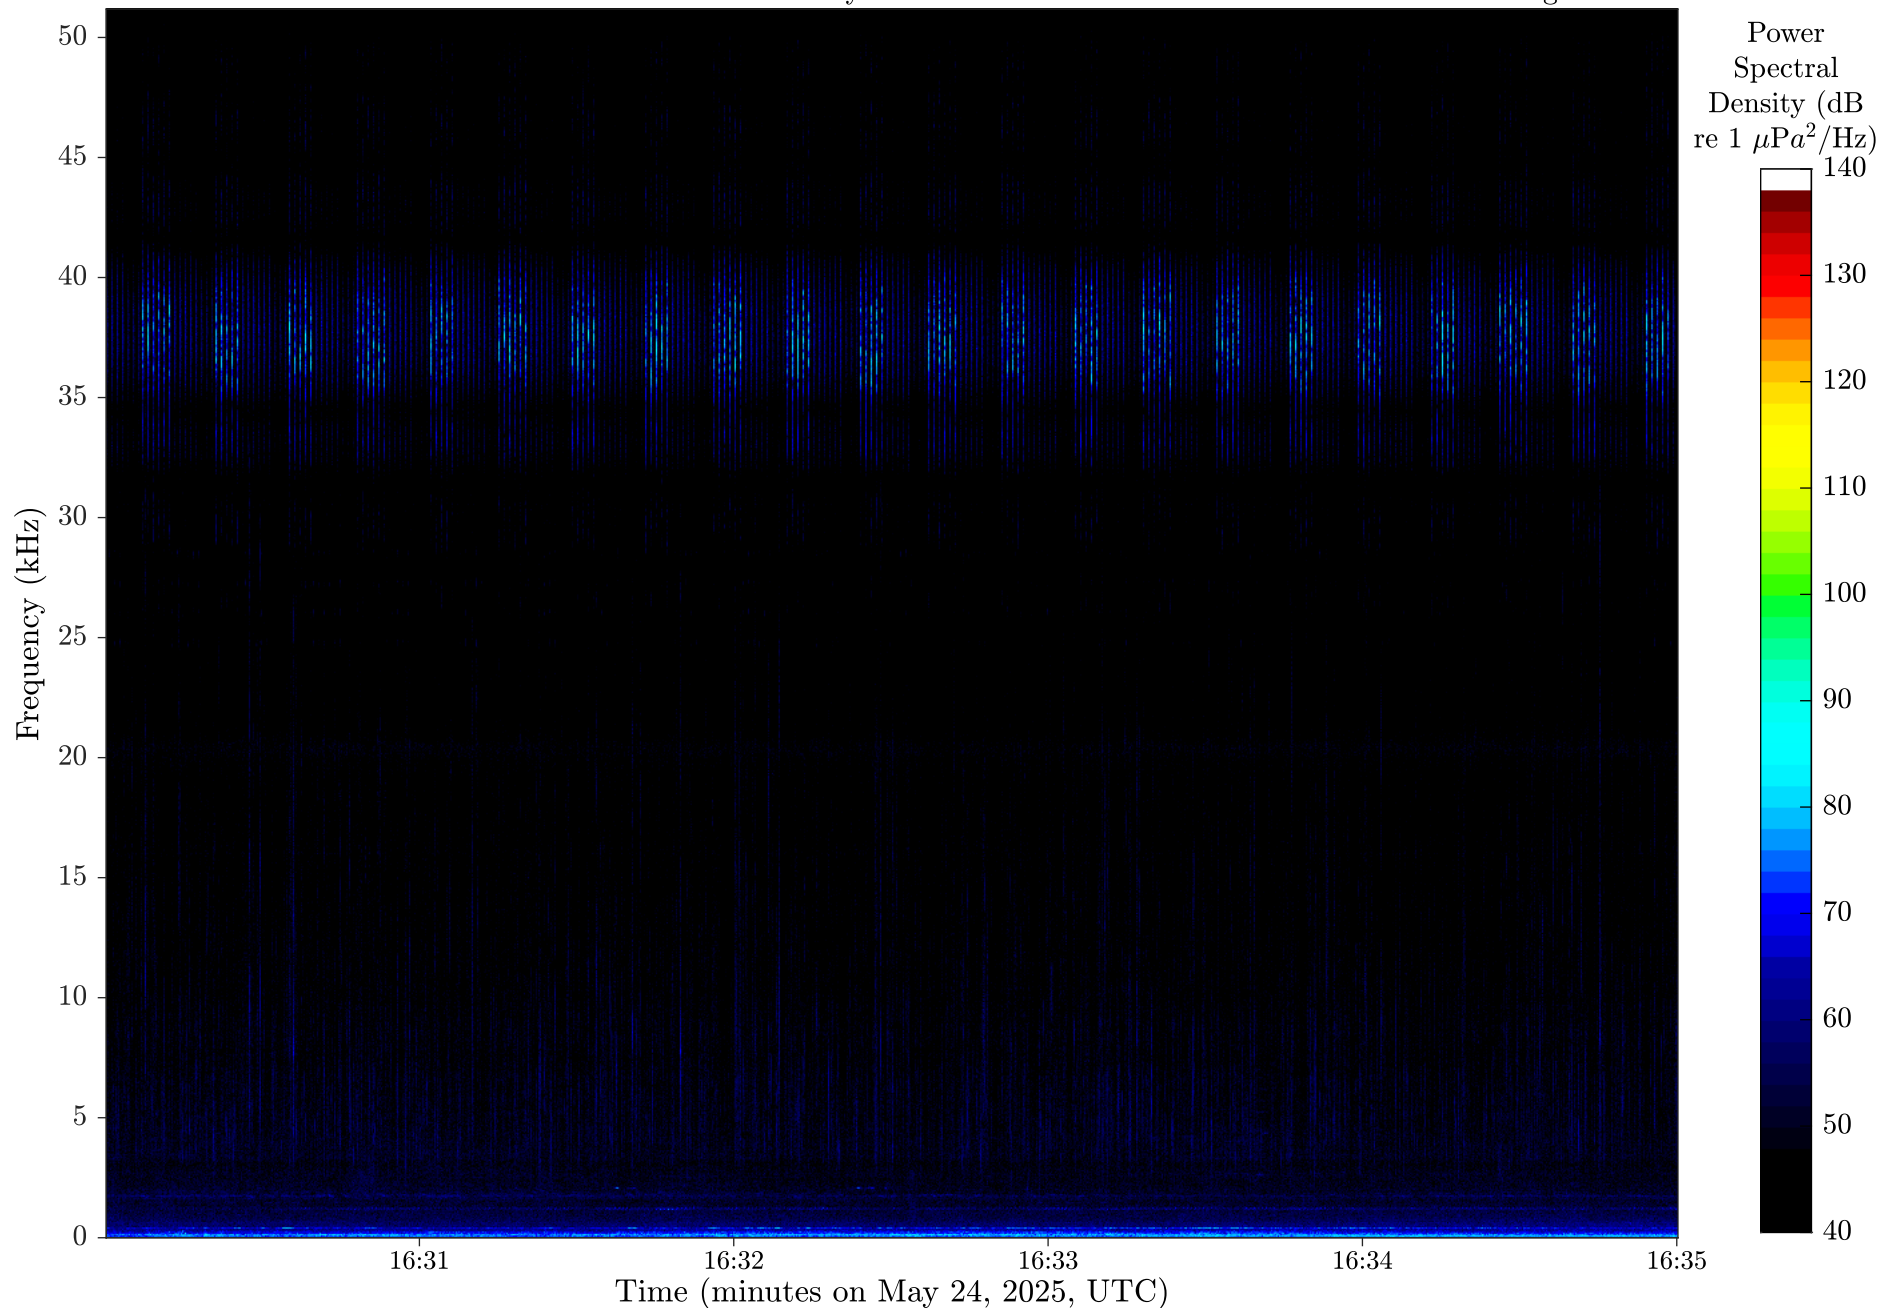


Comments: 31.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:22 UTC

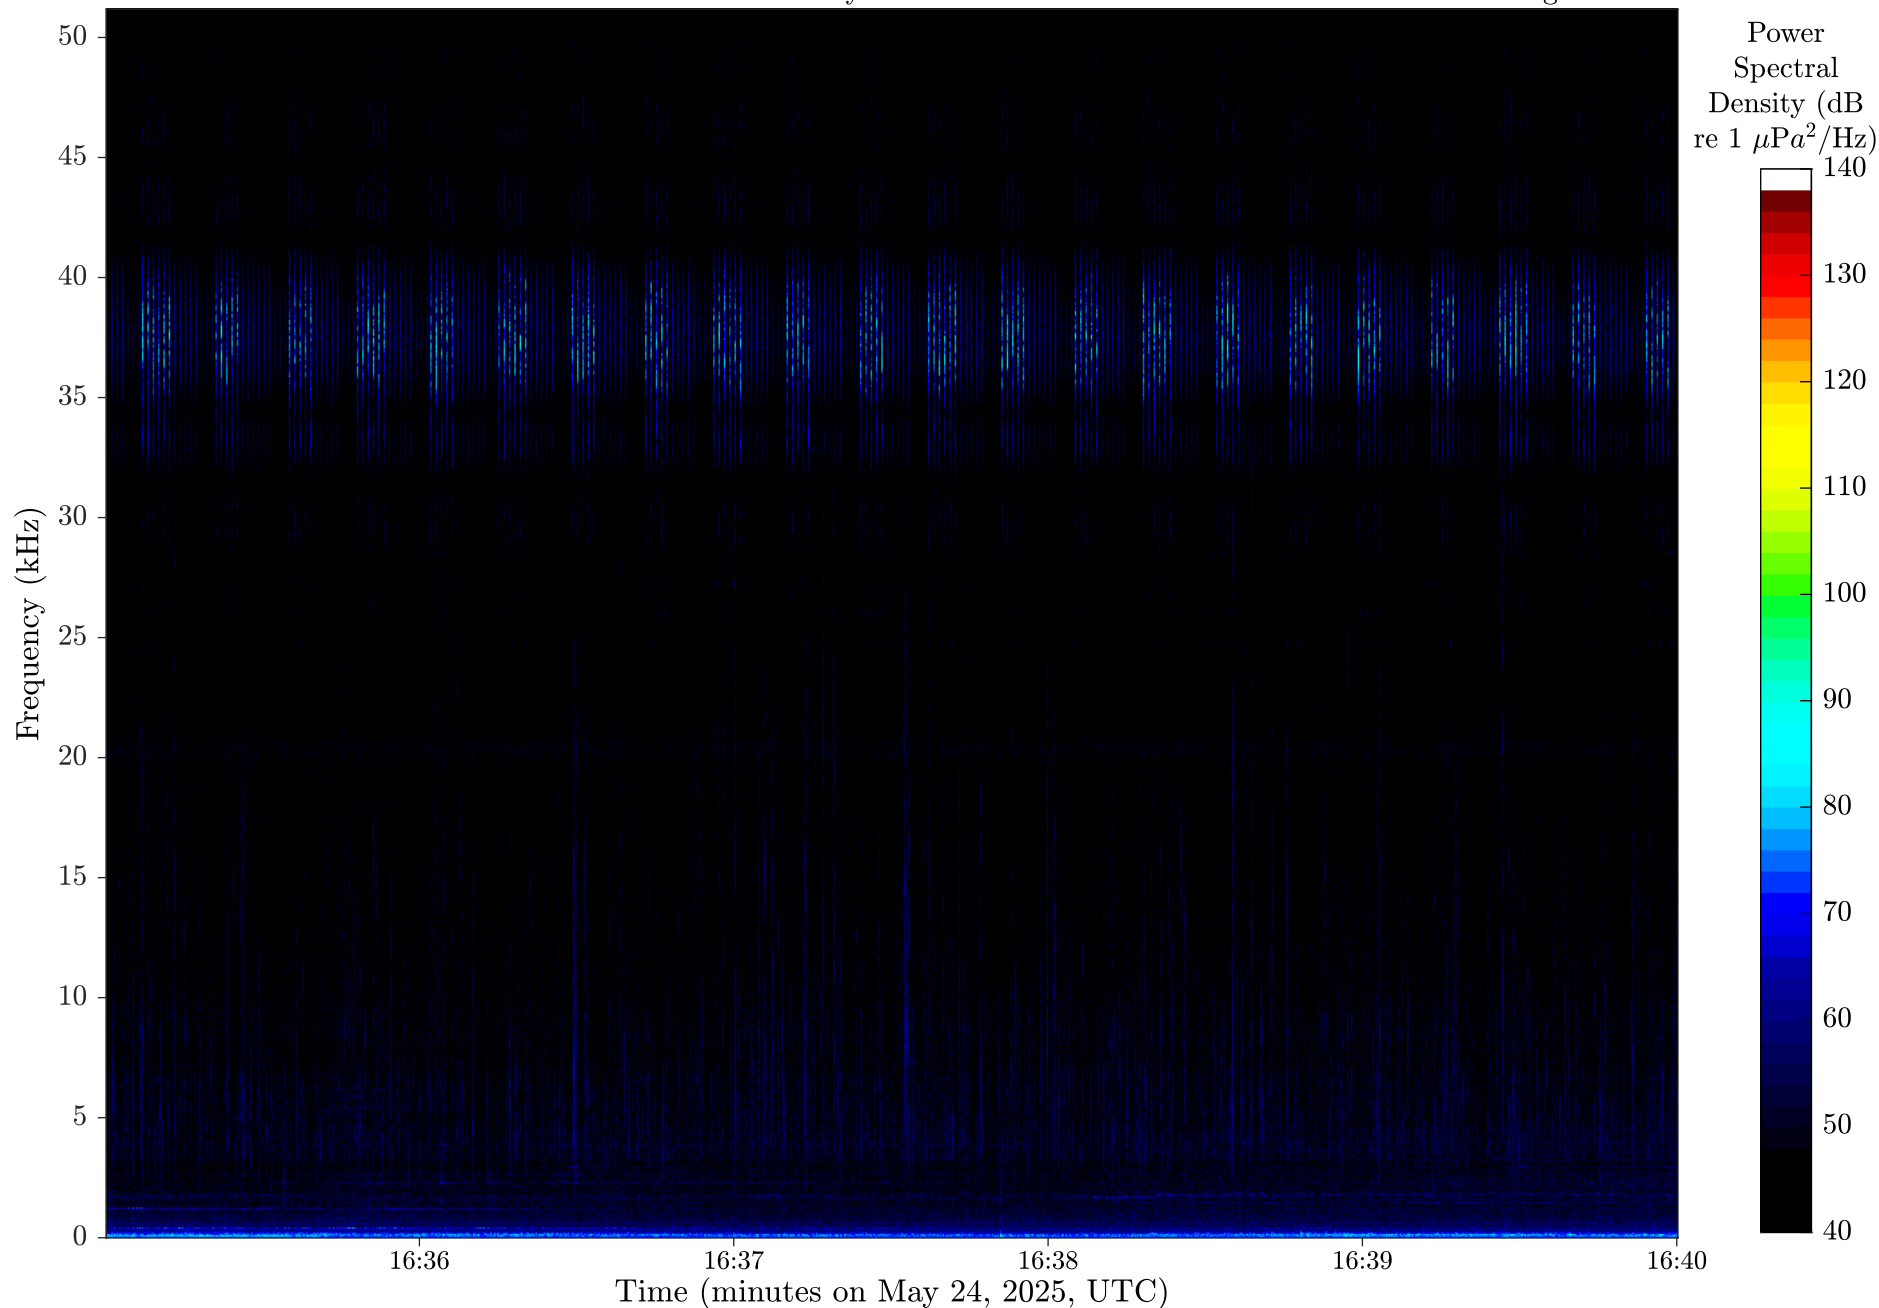


Comments: 30.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:30 UTC

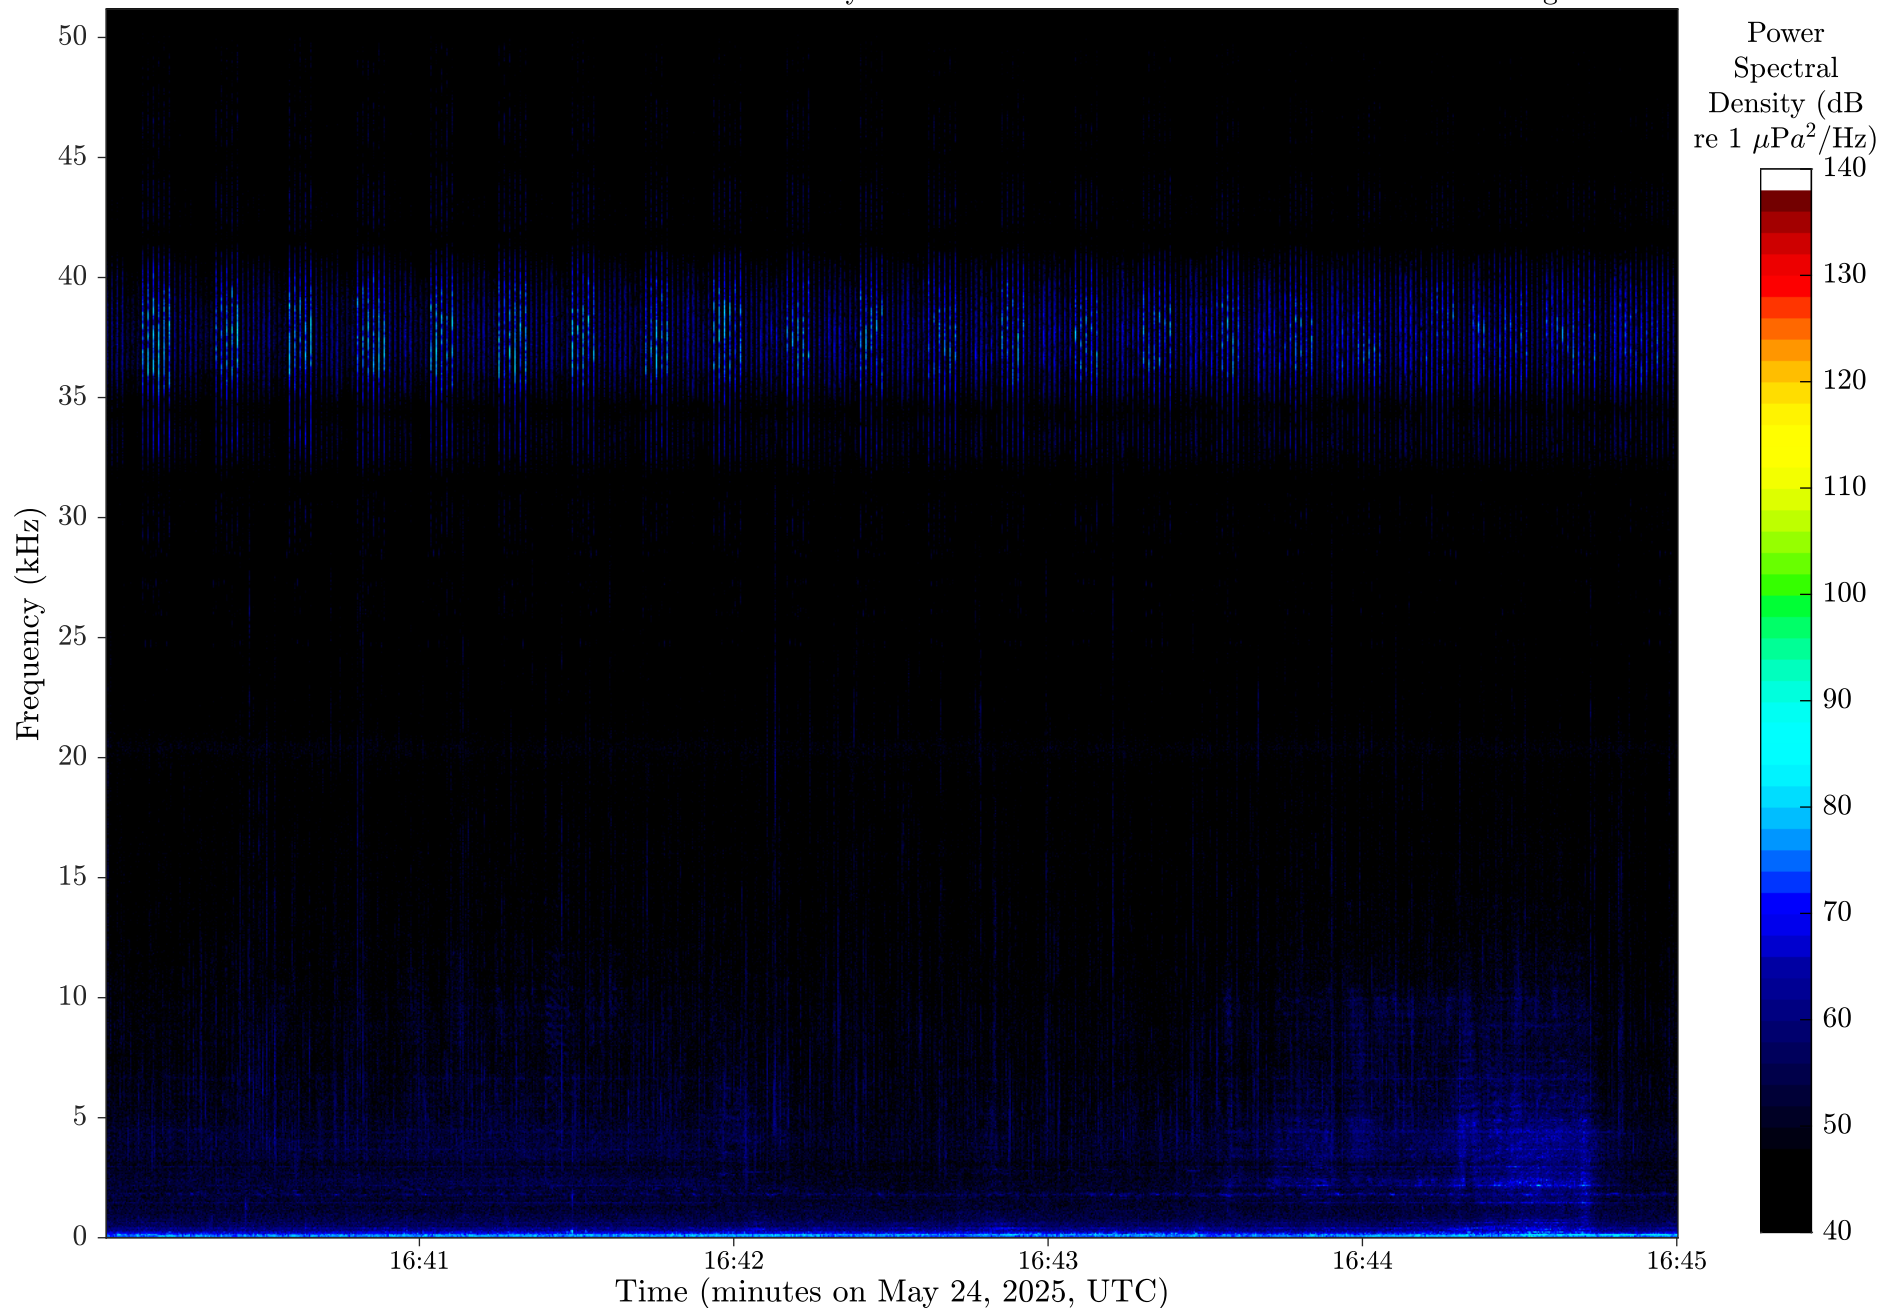


Comments: 29.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:38 UTC

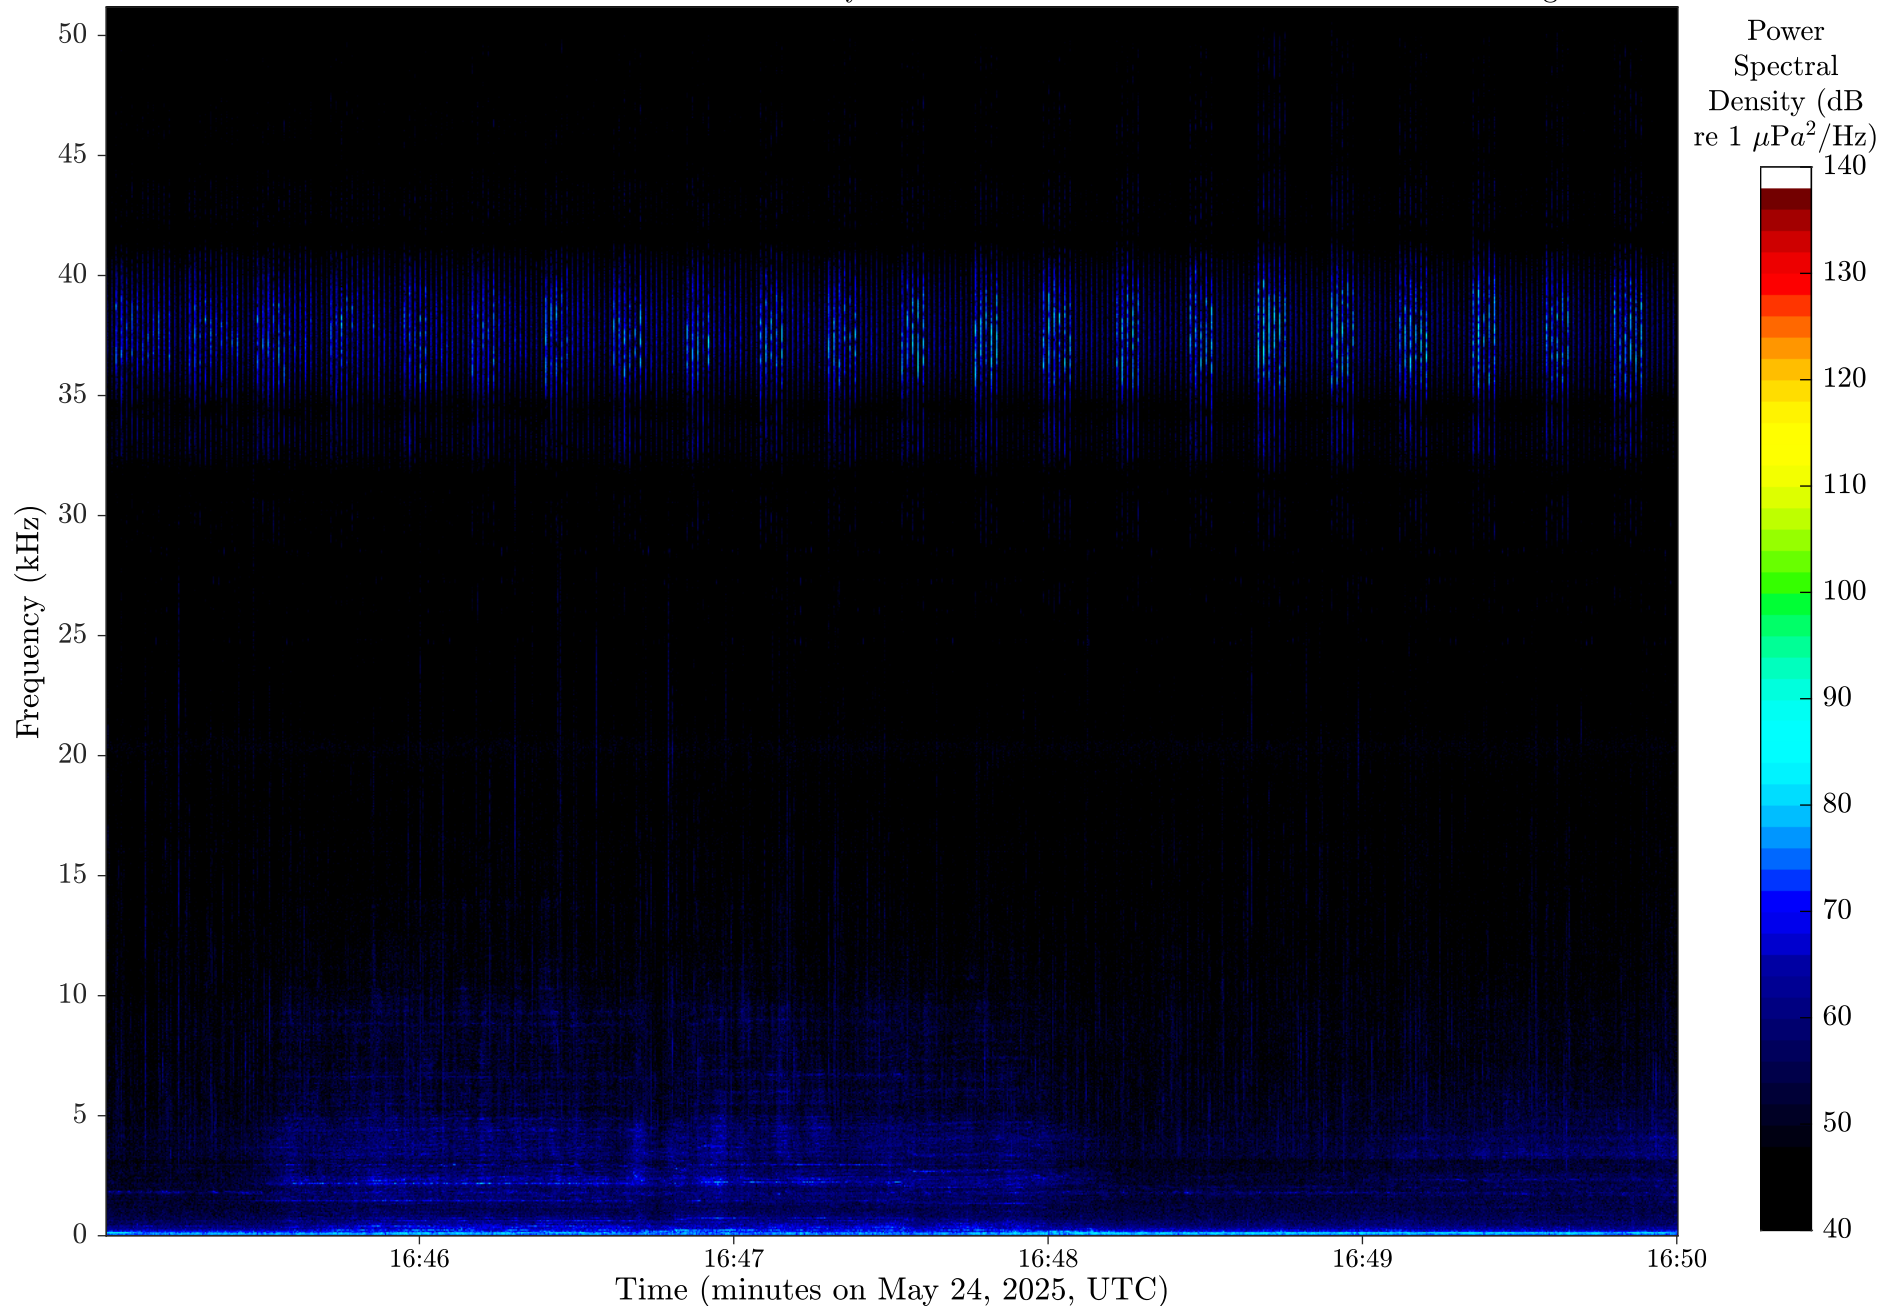


Comments: 29.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:46 UTC

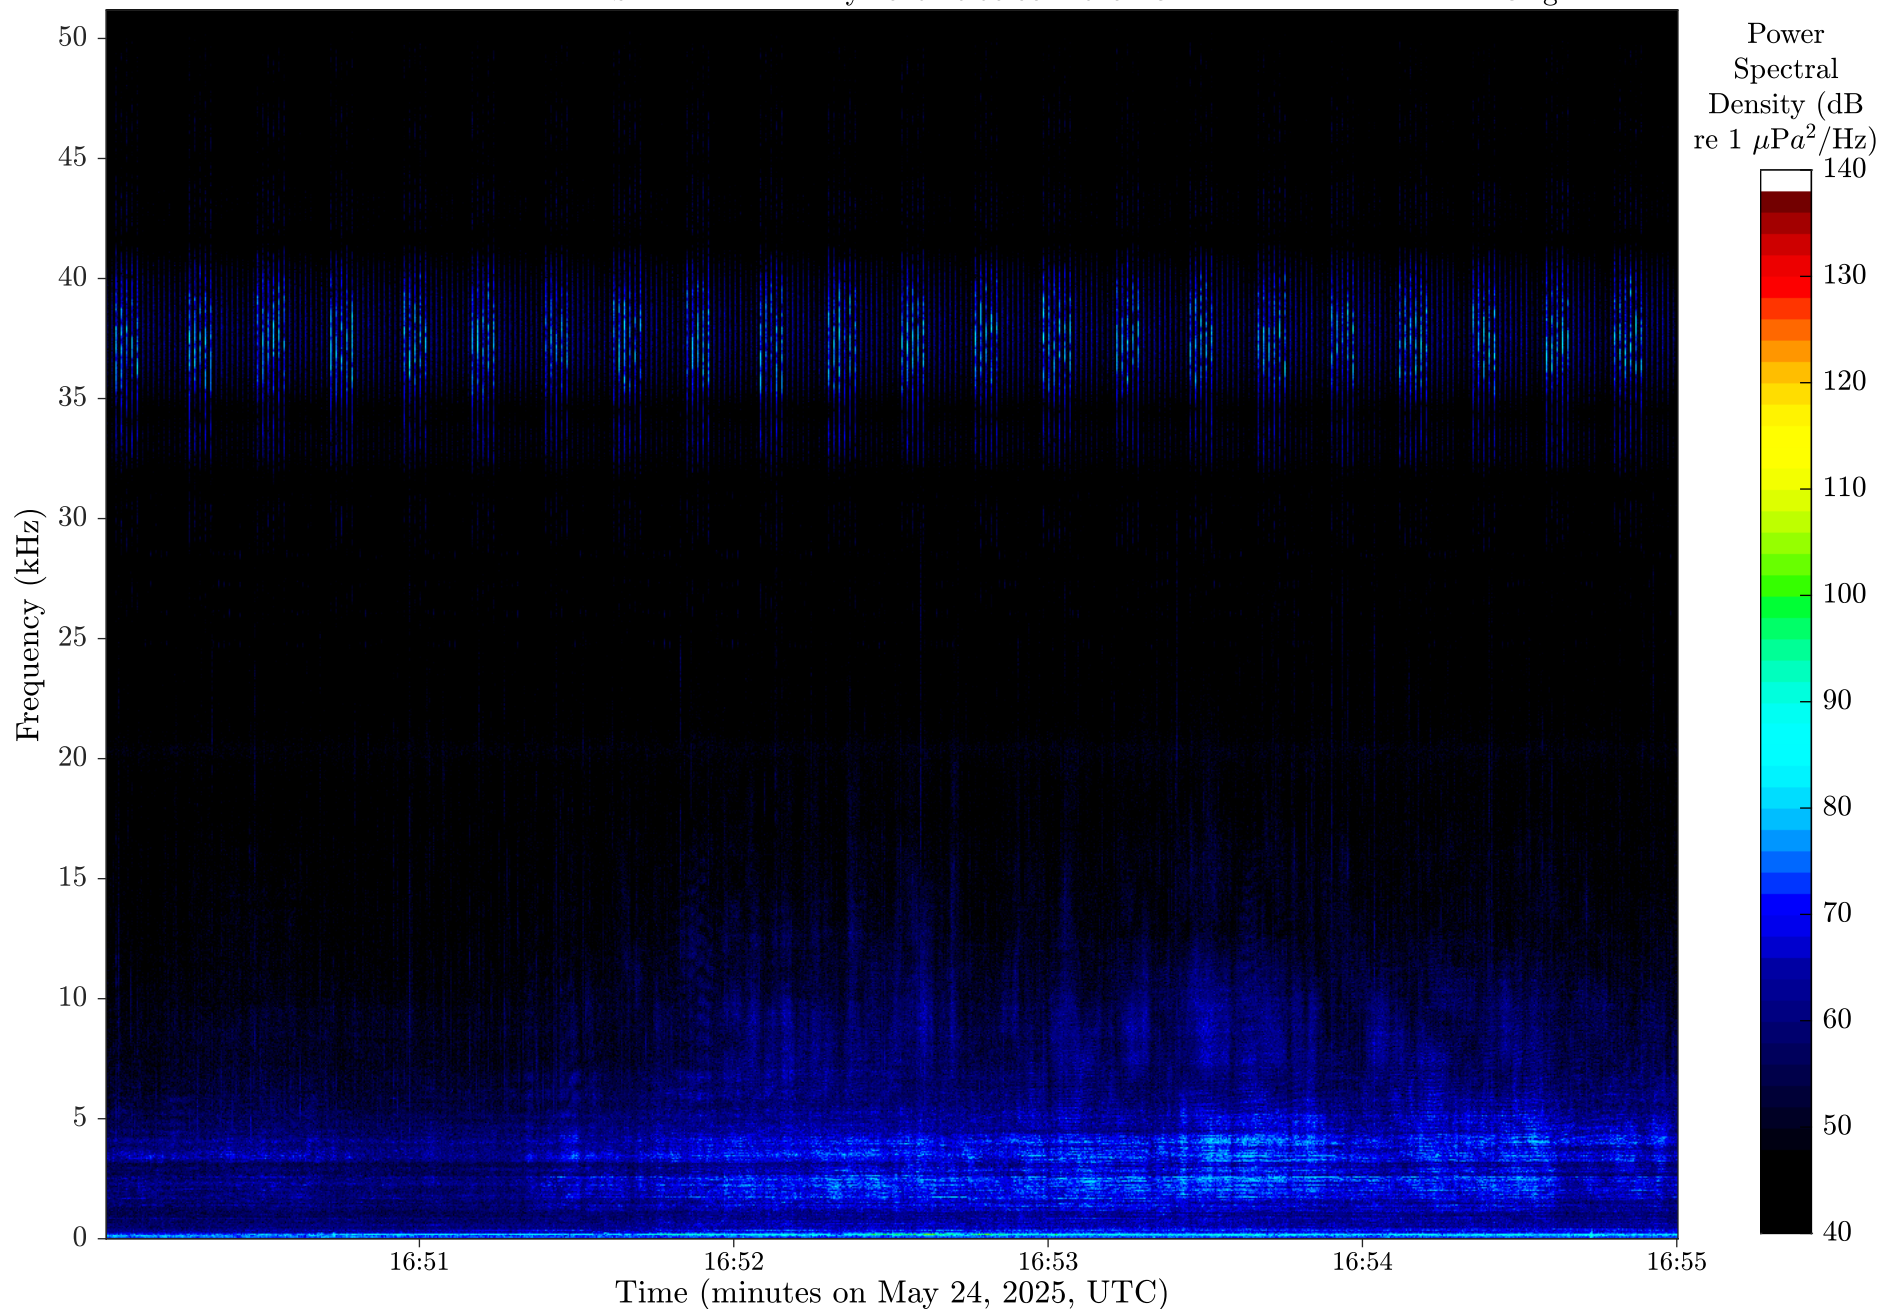


Comments: 26.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:54 UTC

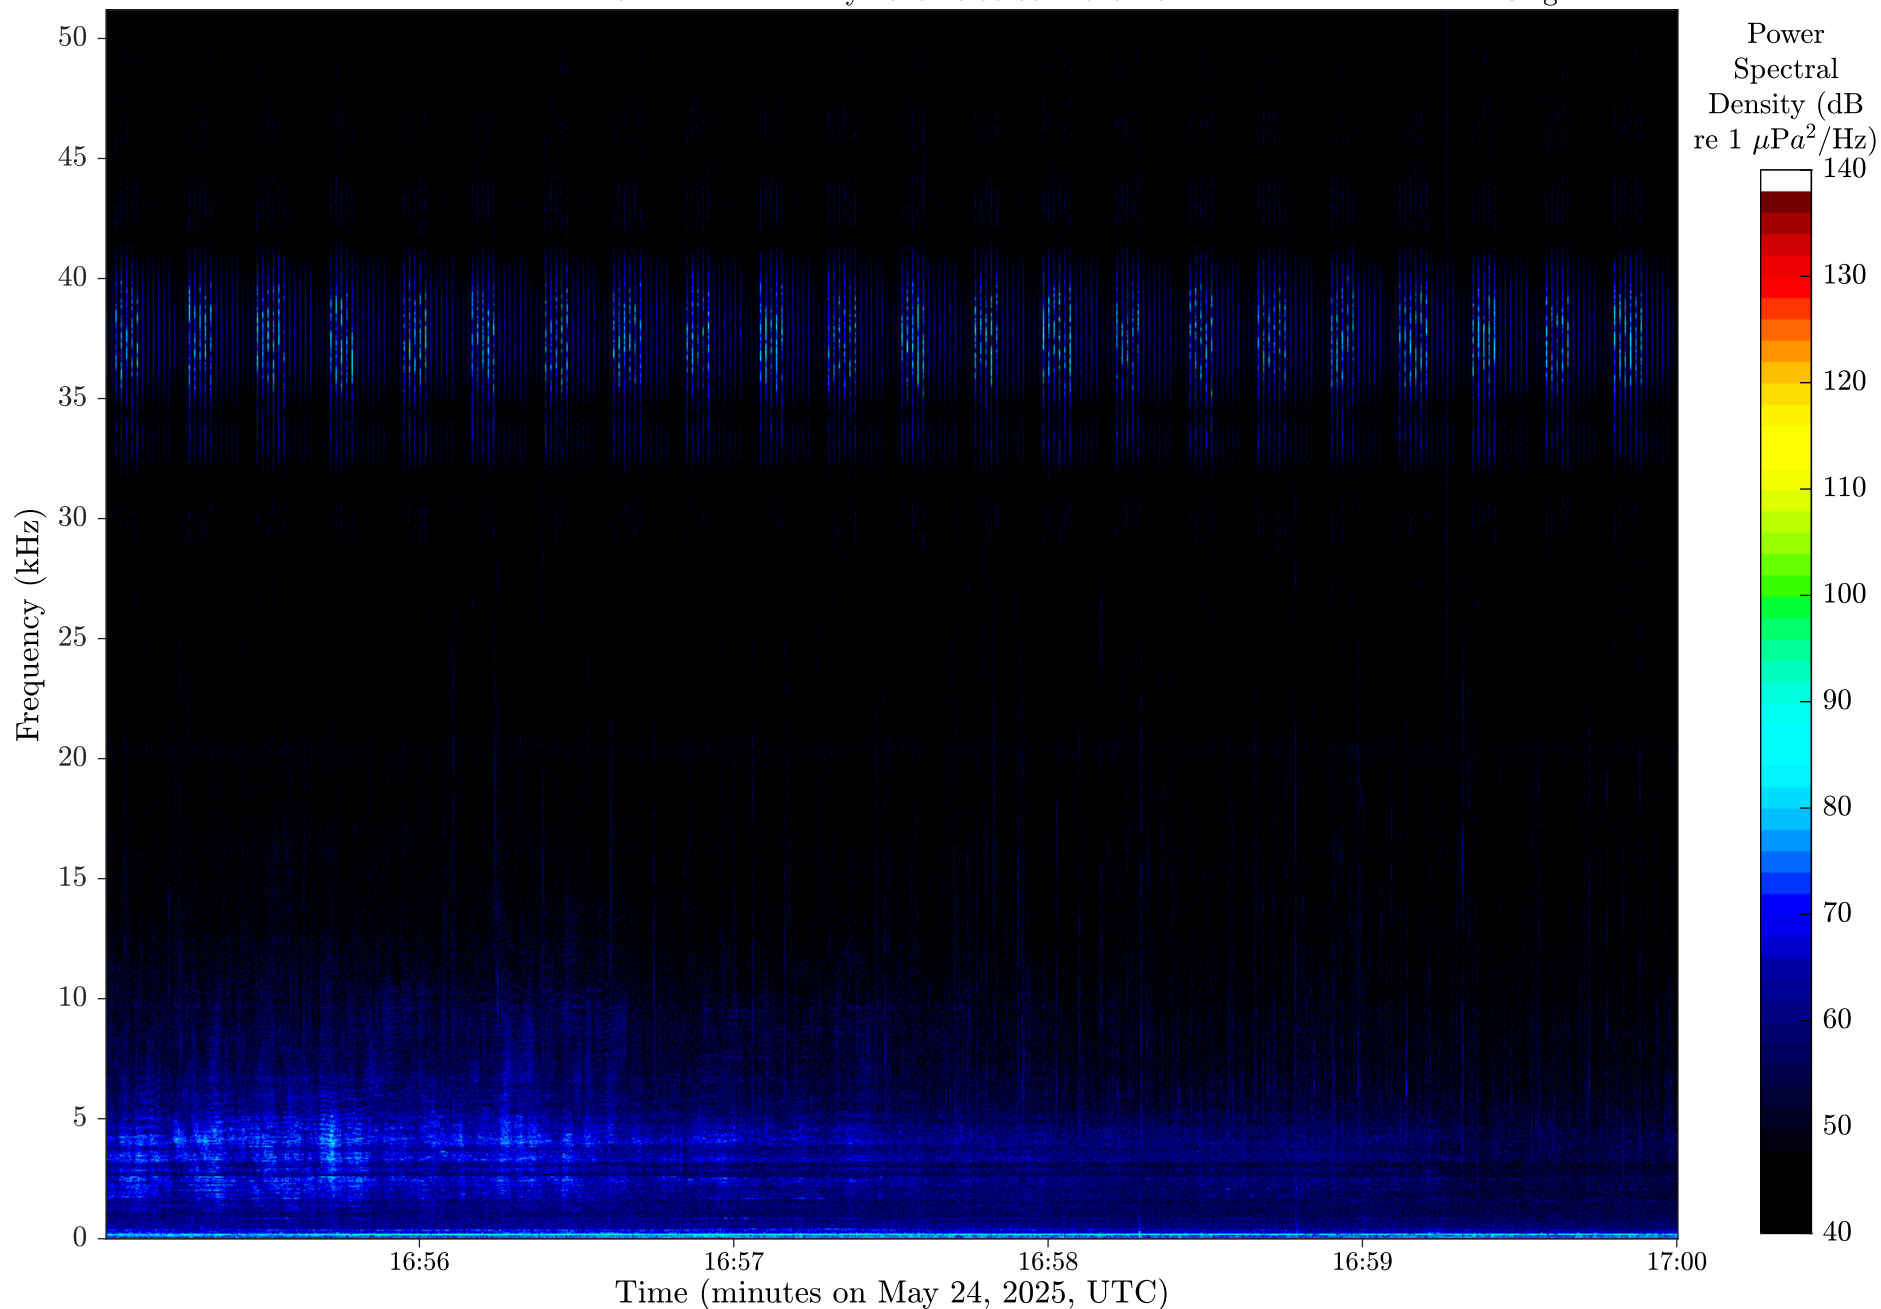


Comments: 28.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:35:02 UTC

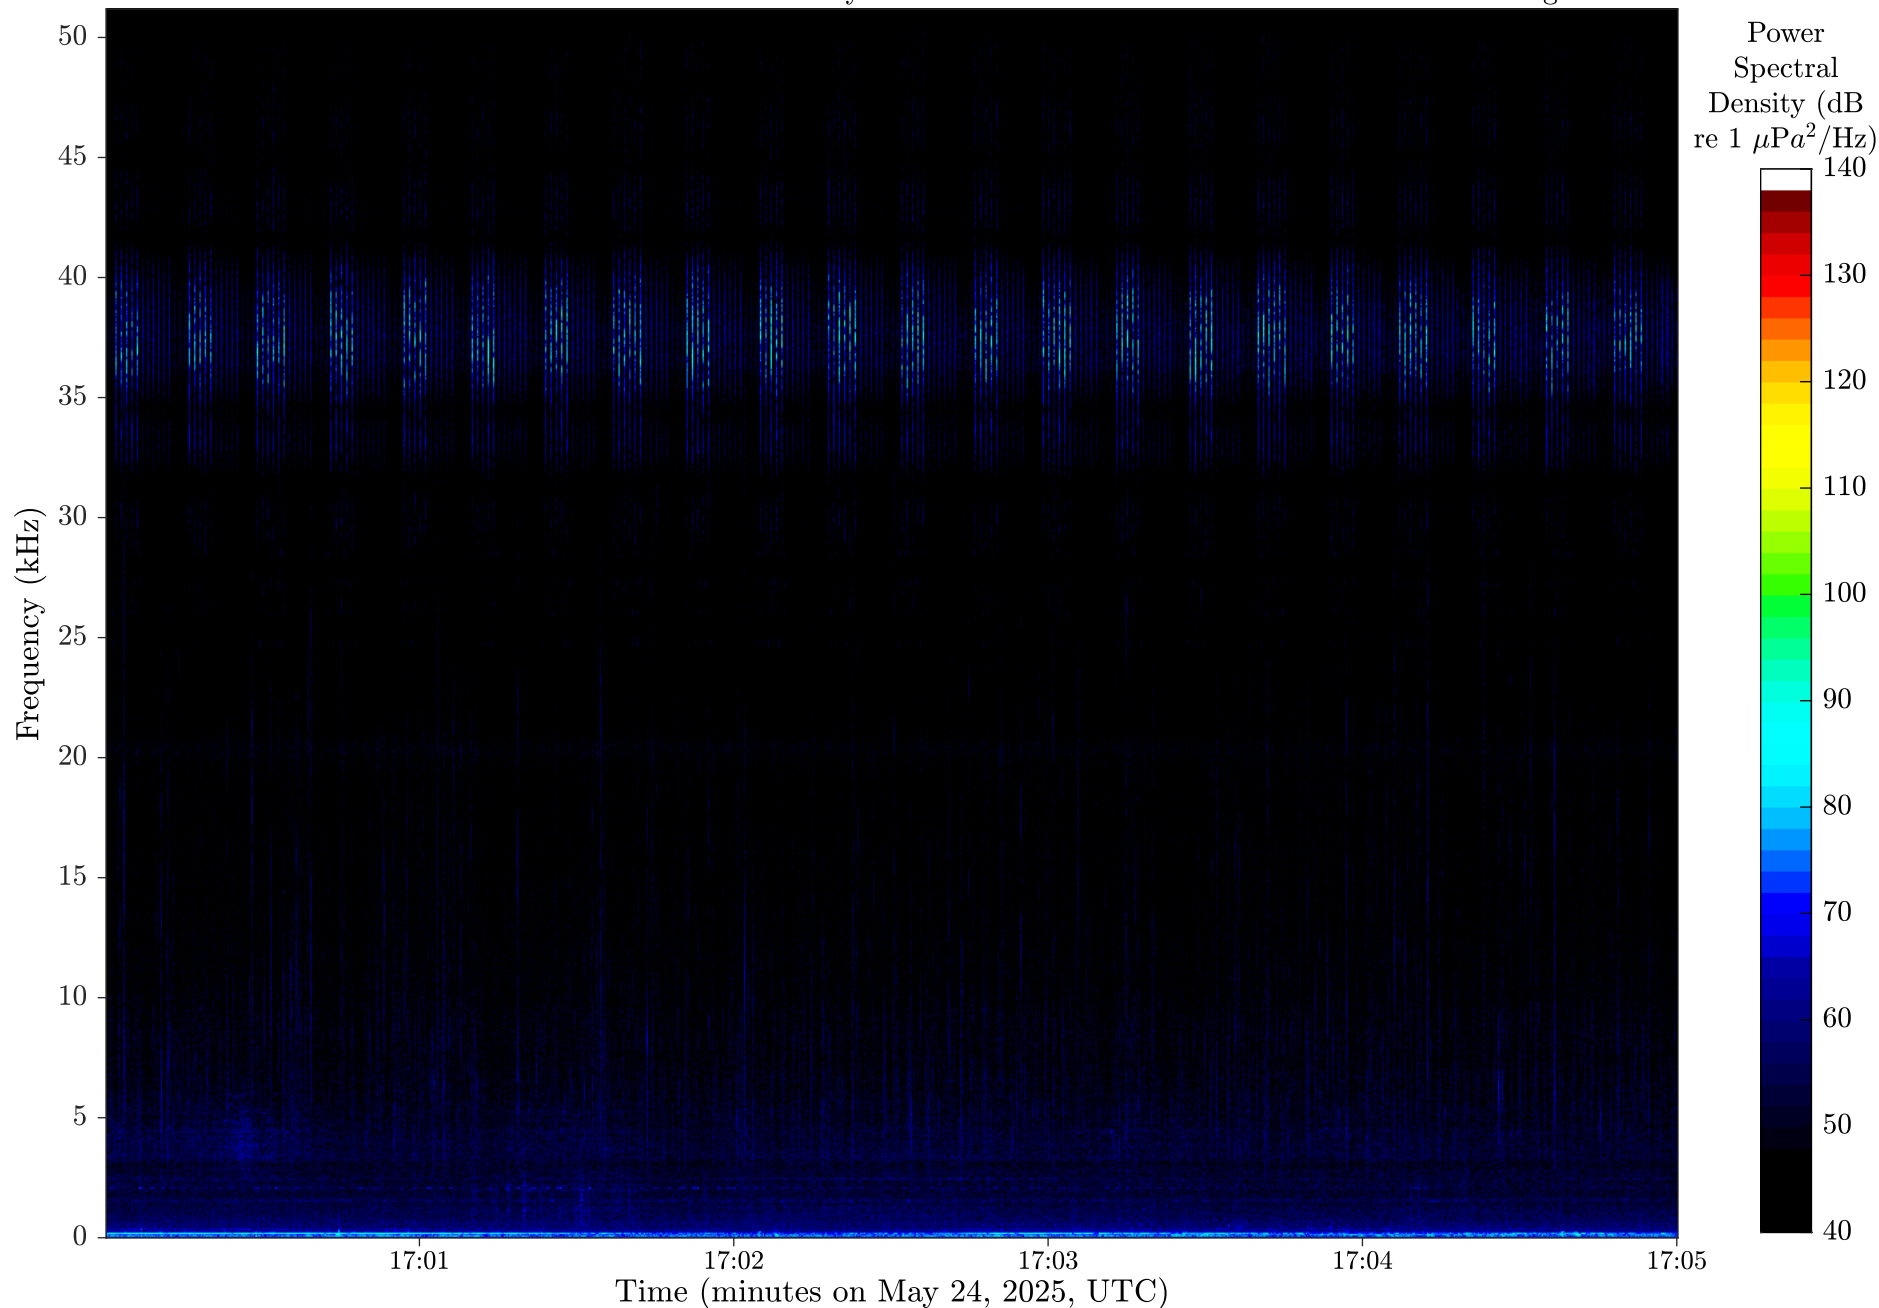

Comments: 28.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:35:10 UTC

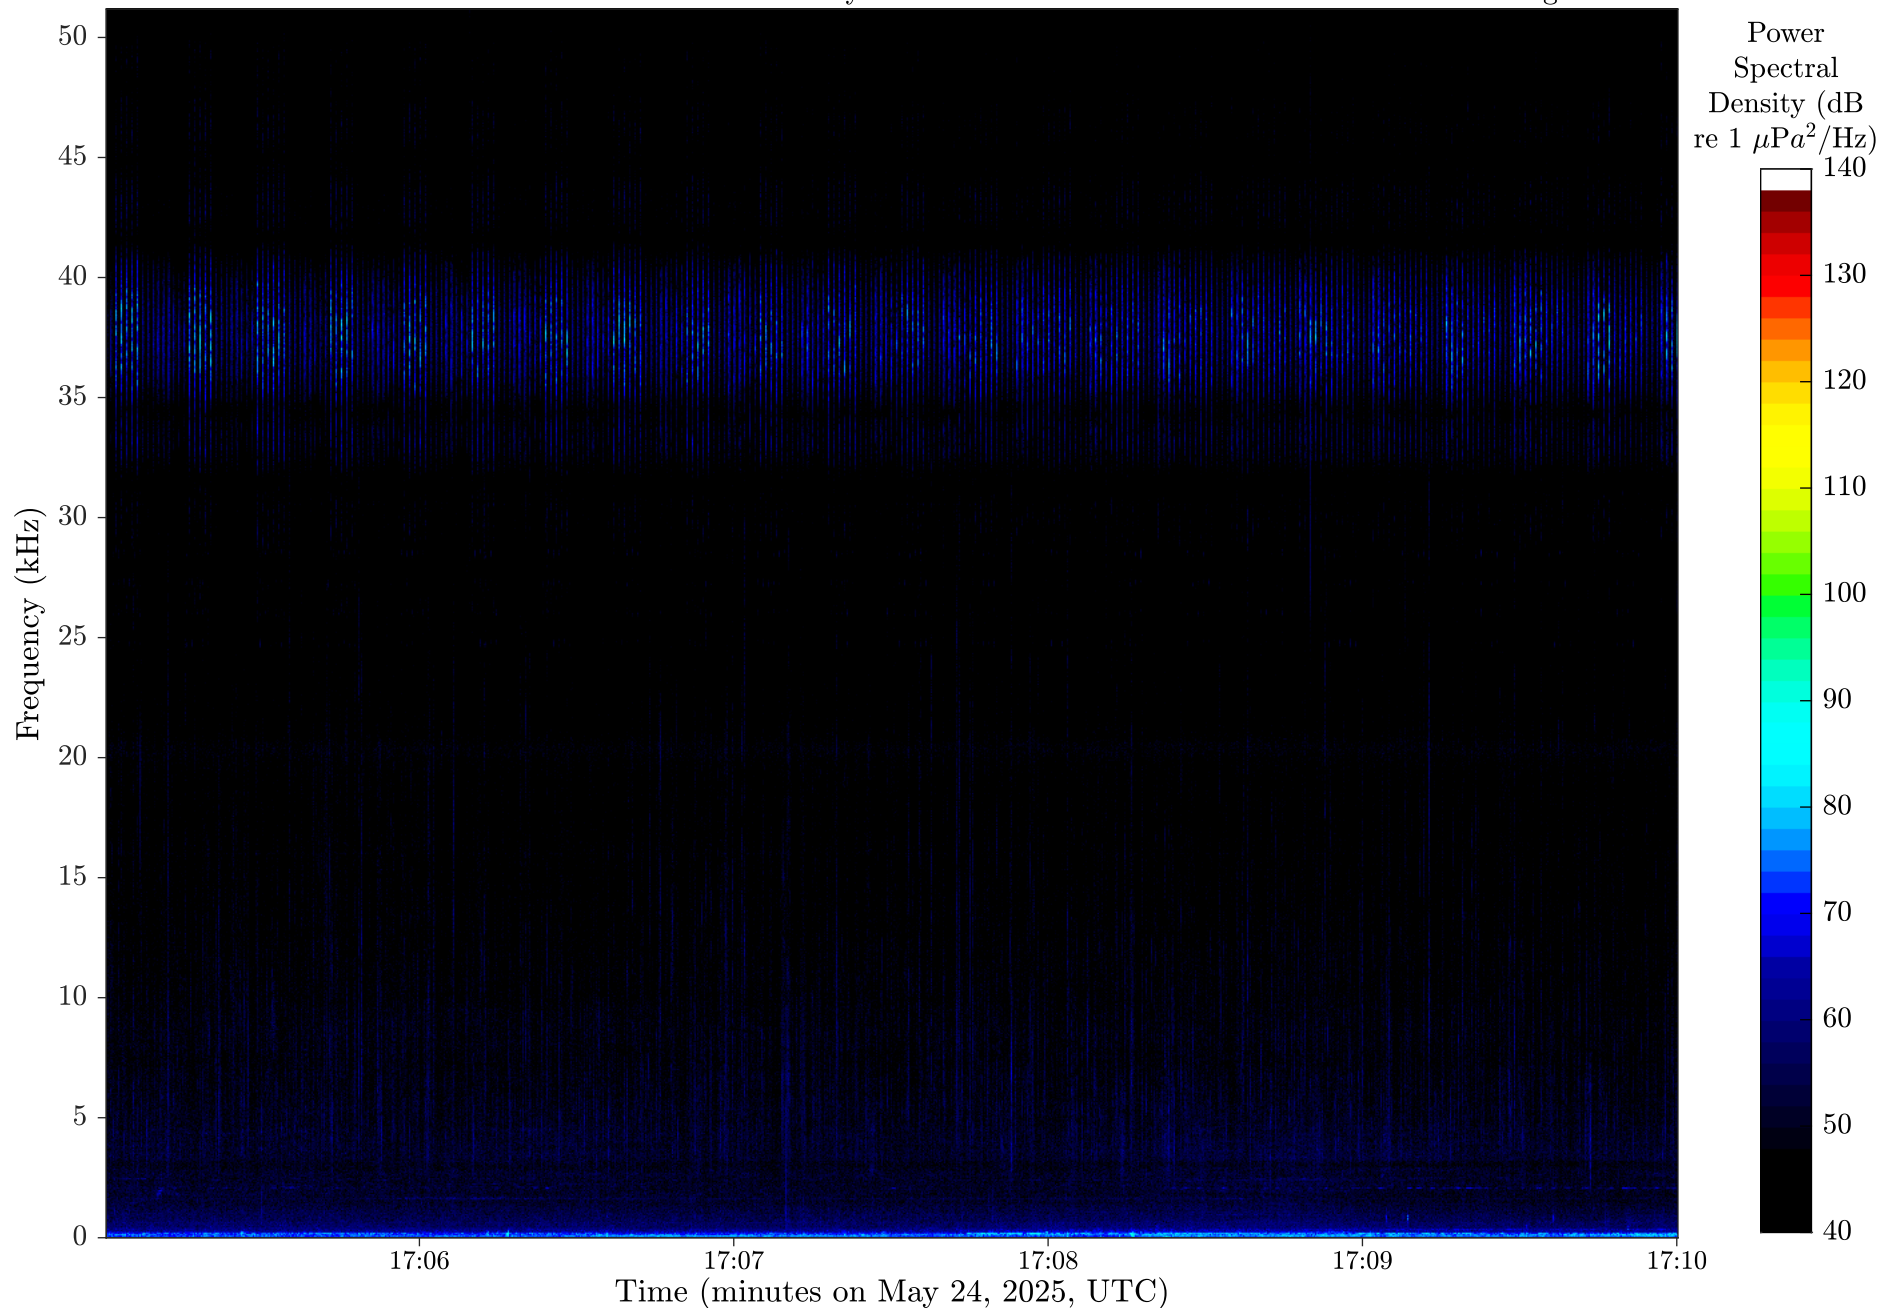

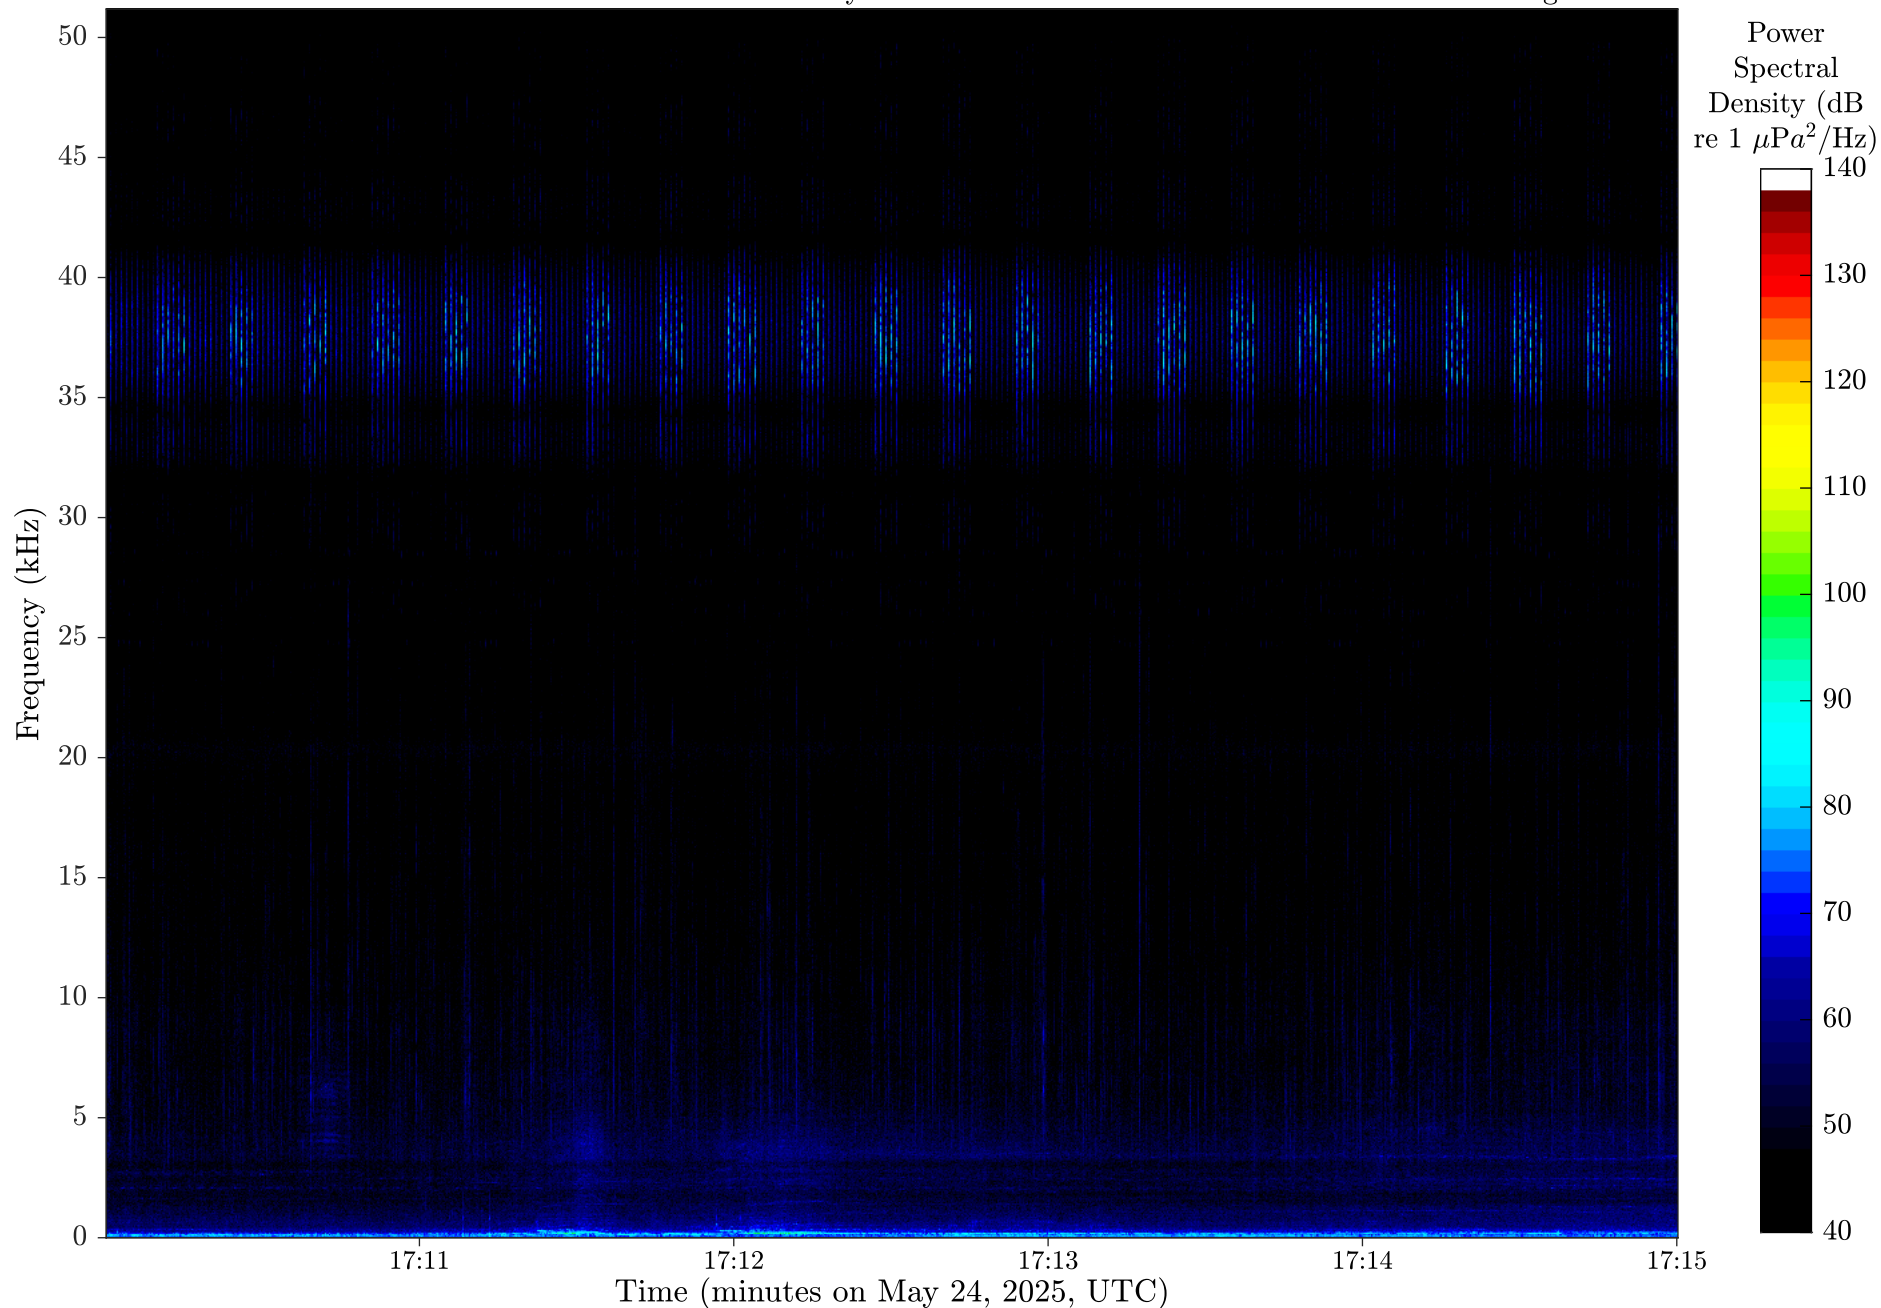


Comments: 30.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:26 UTC

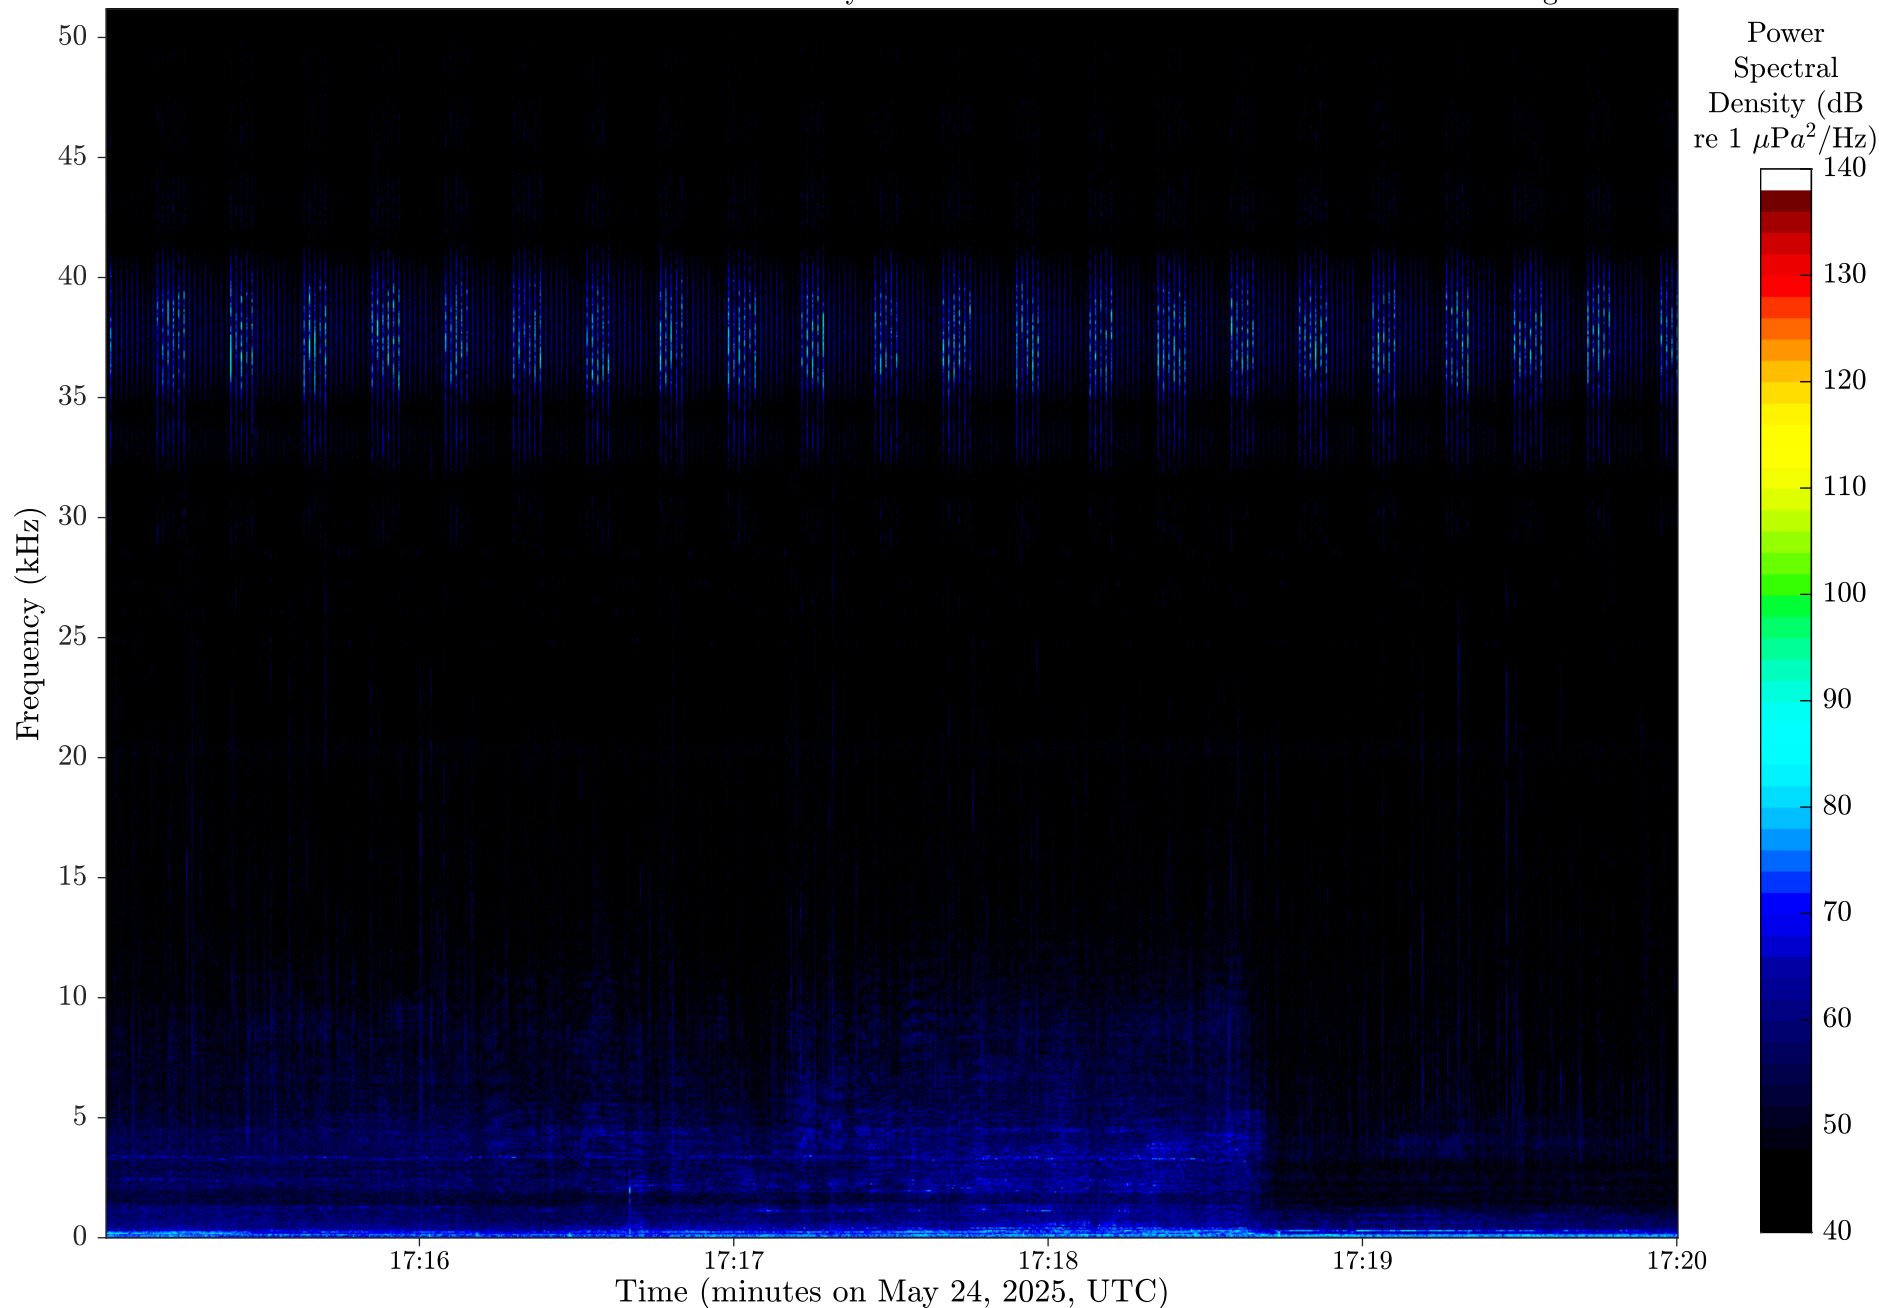


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:35:34 UTC

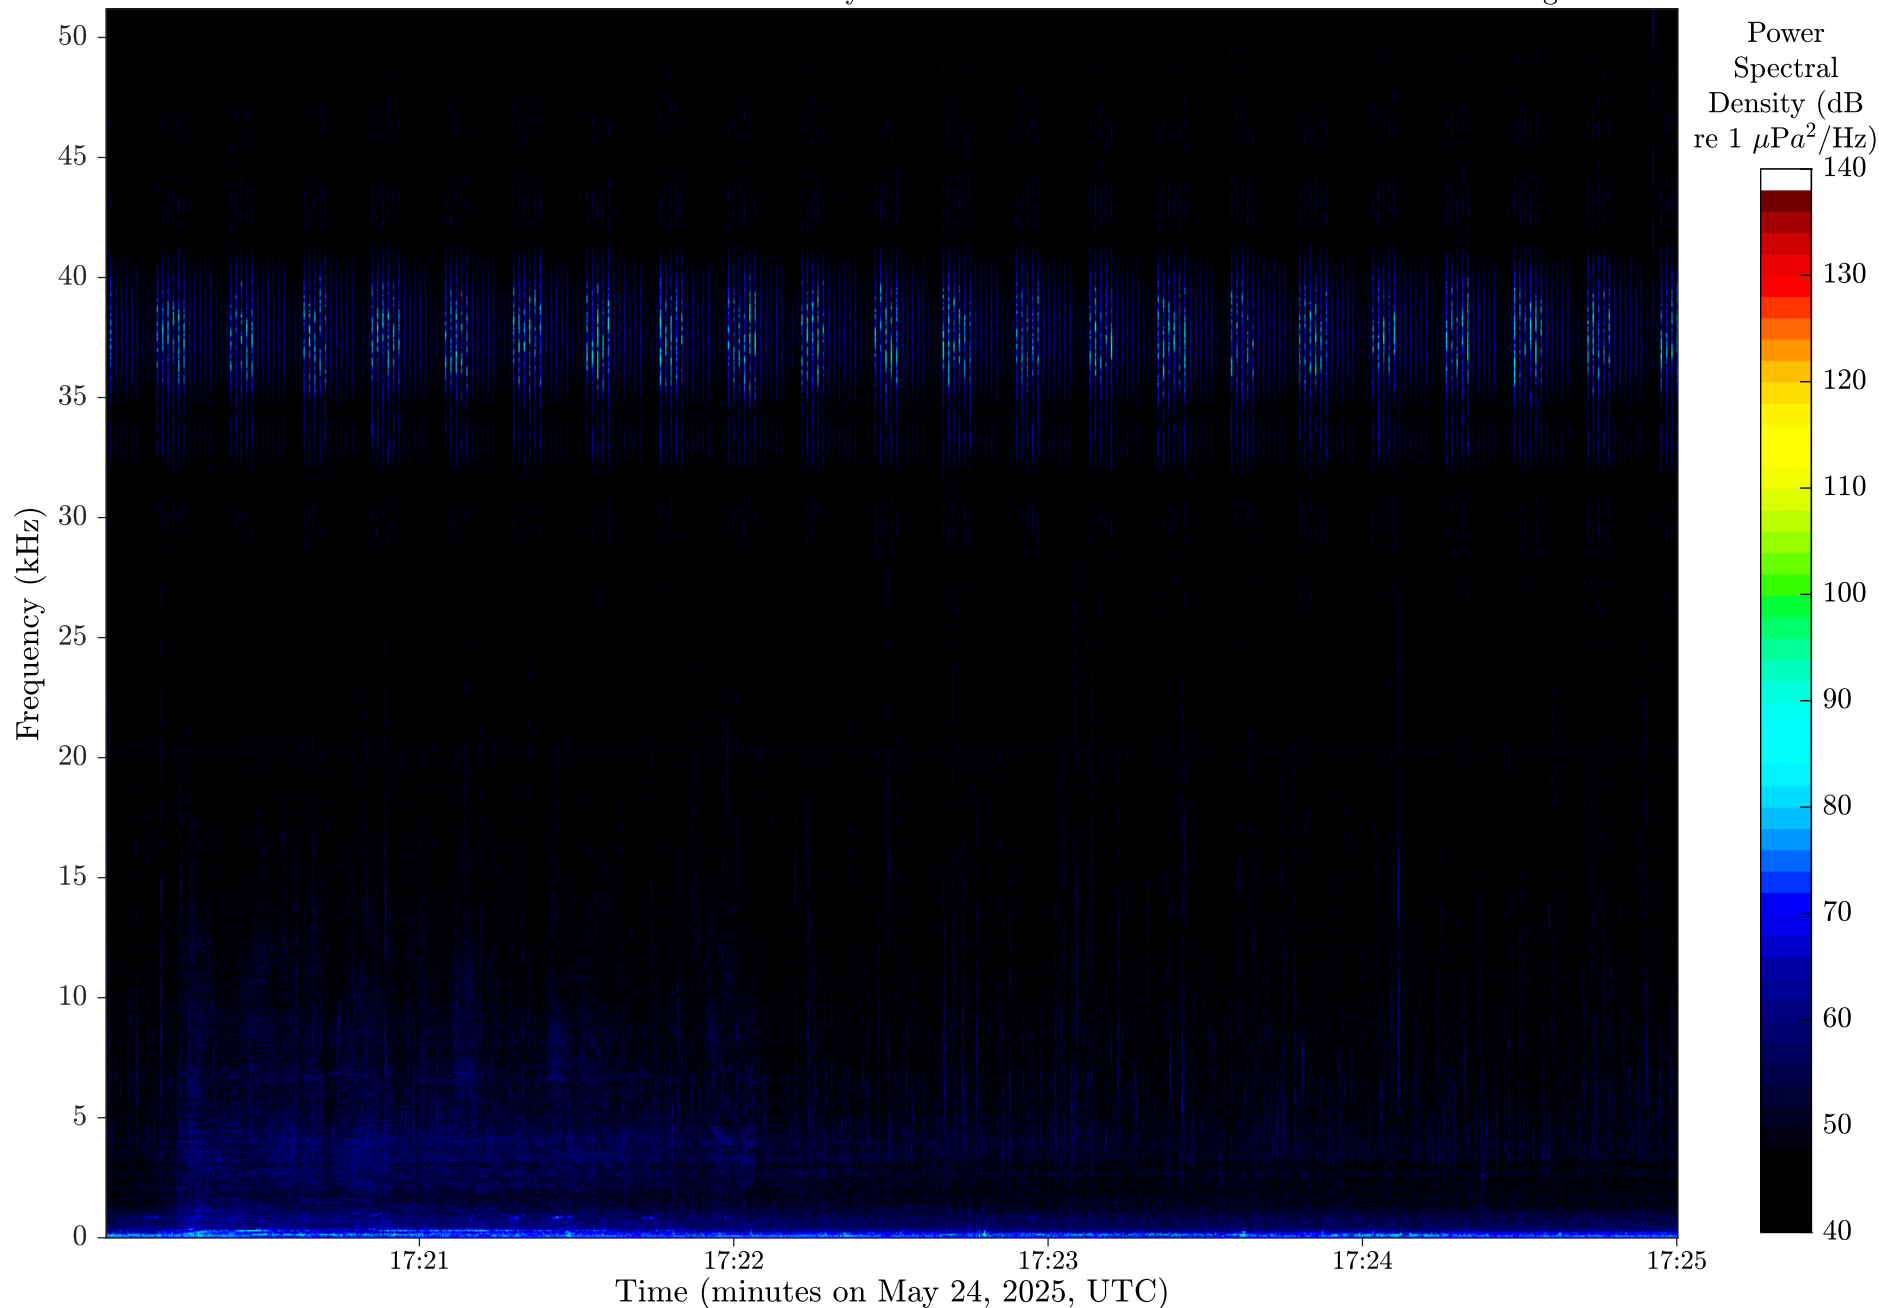

Comments: 32.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:35:42 UTC

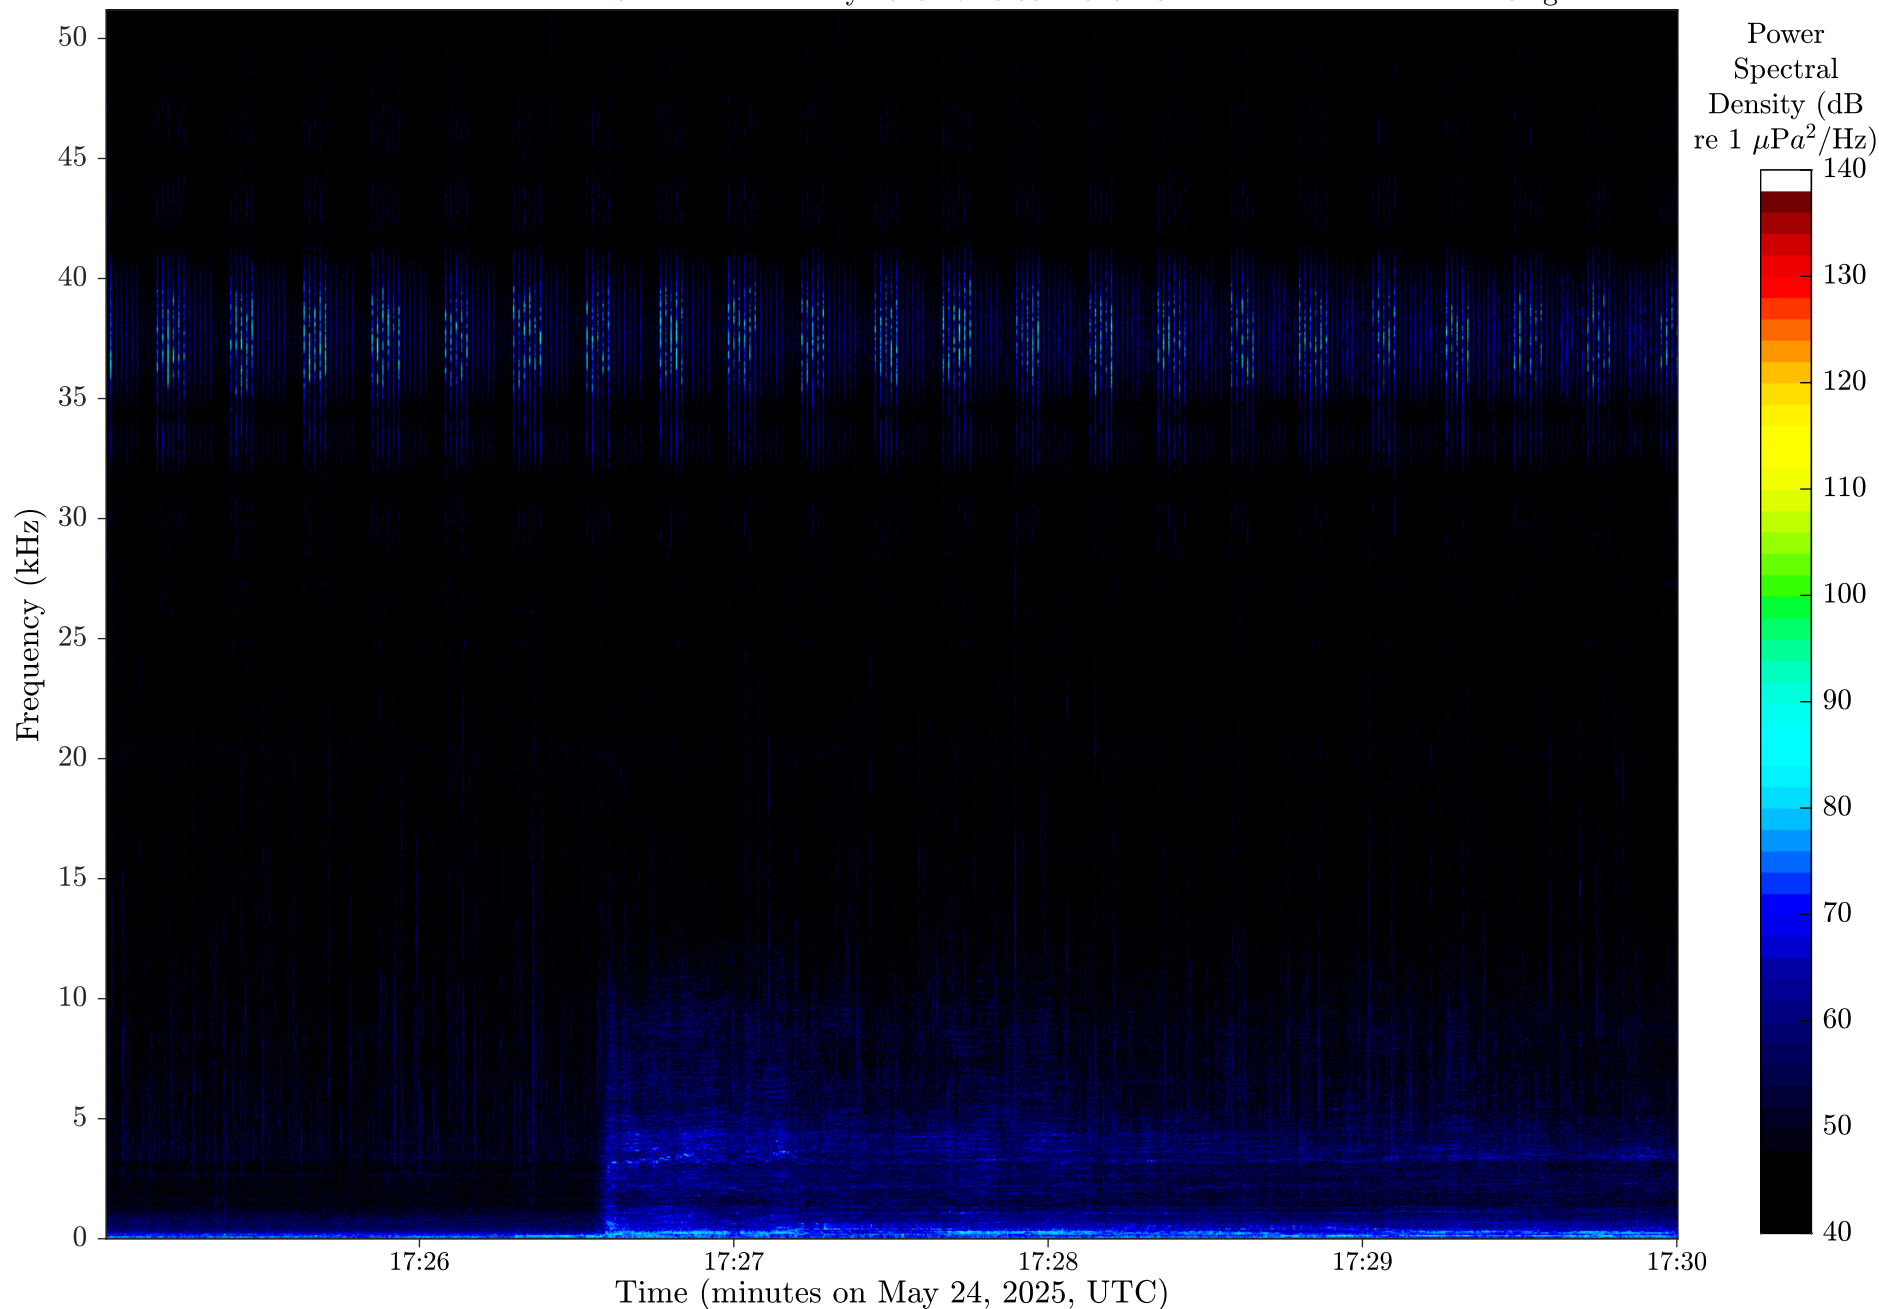

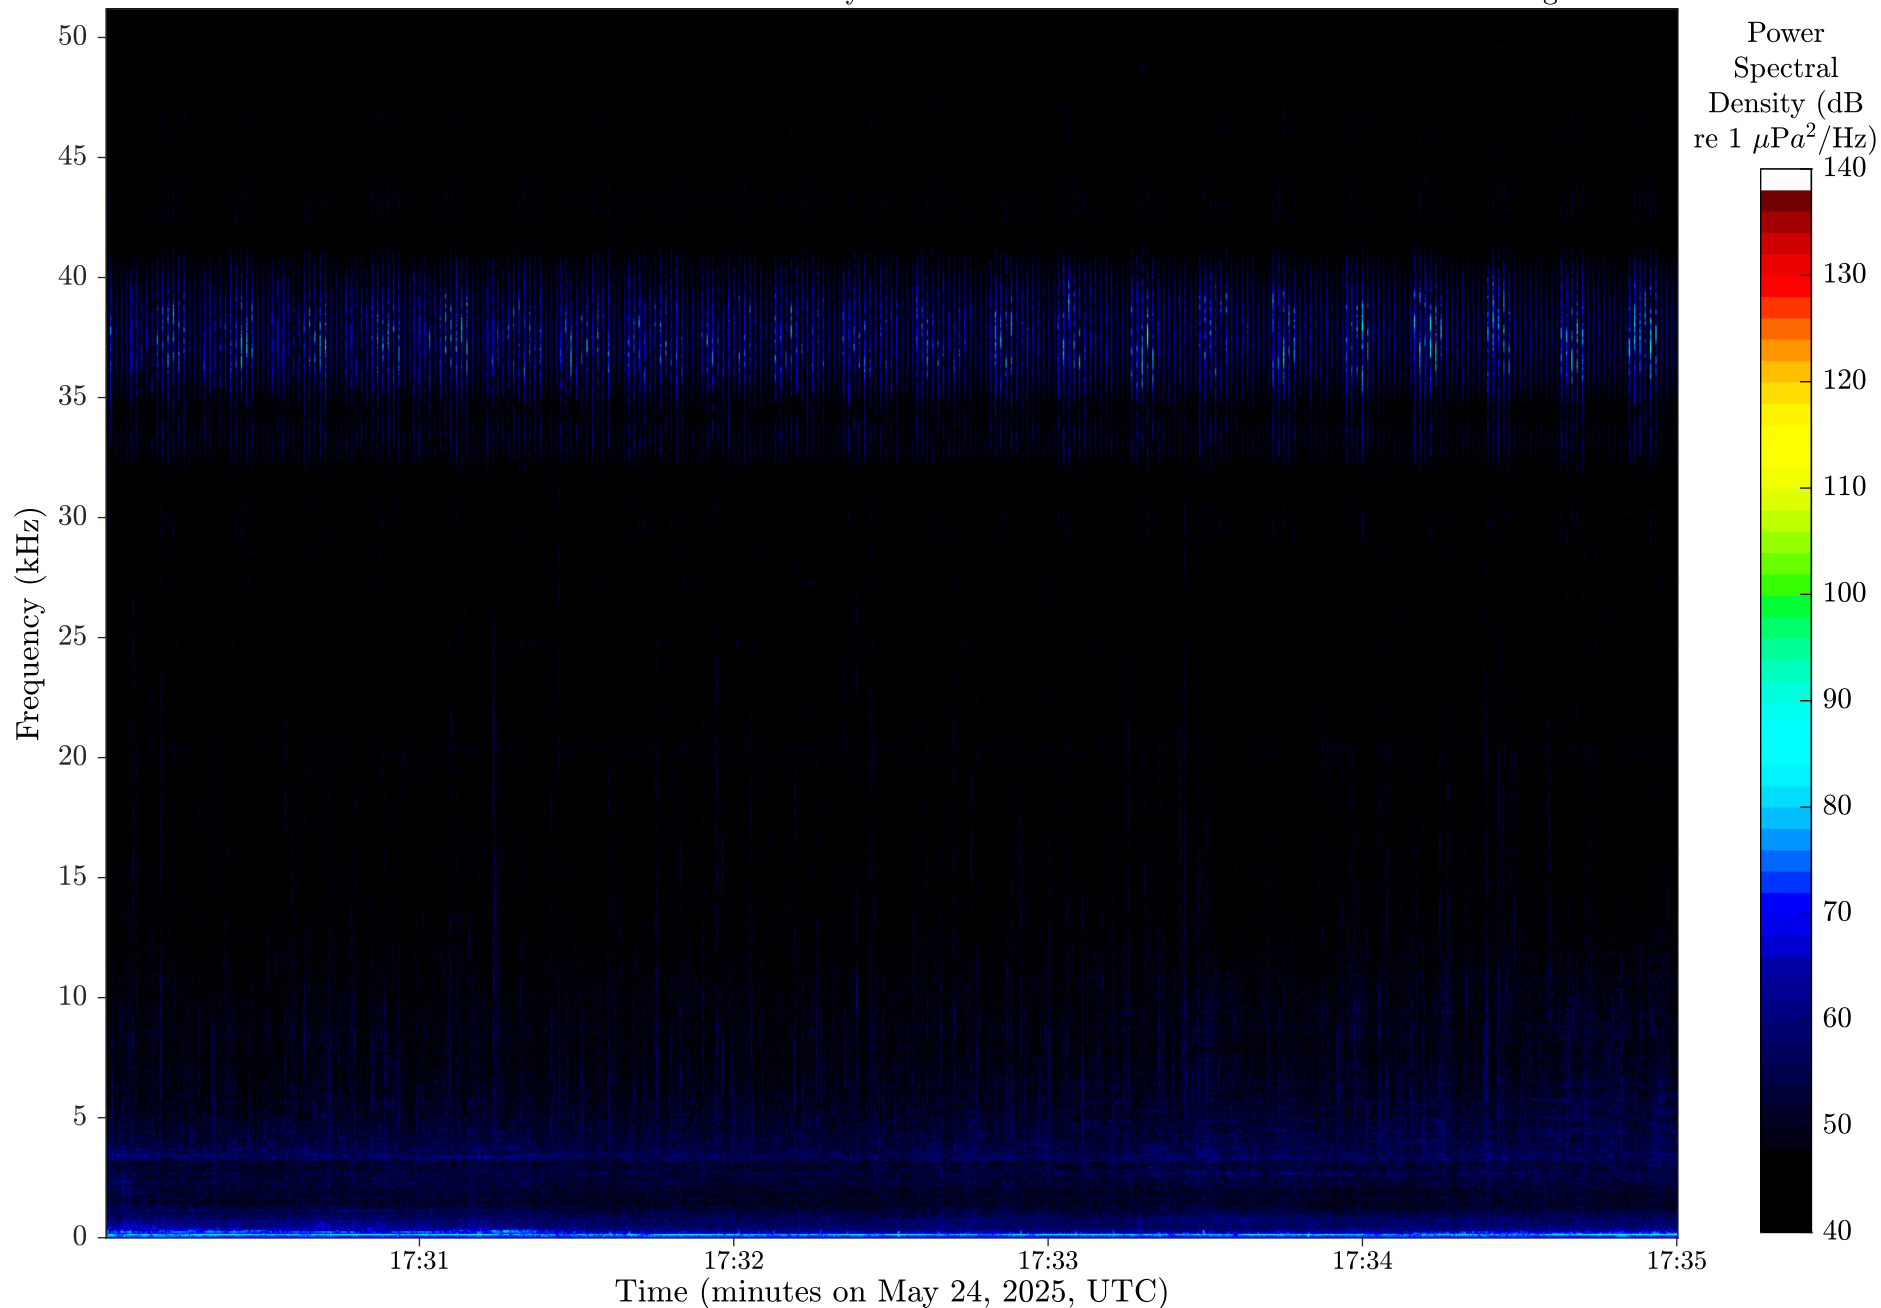


Comments: 31.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:57 UTC

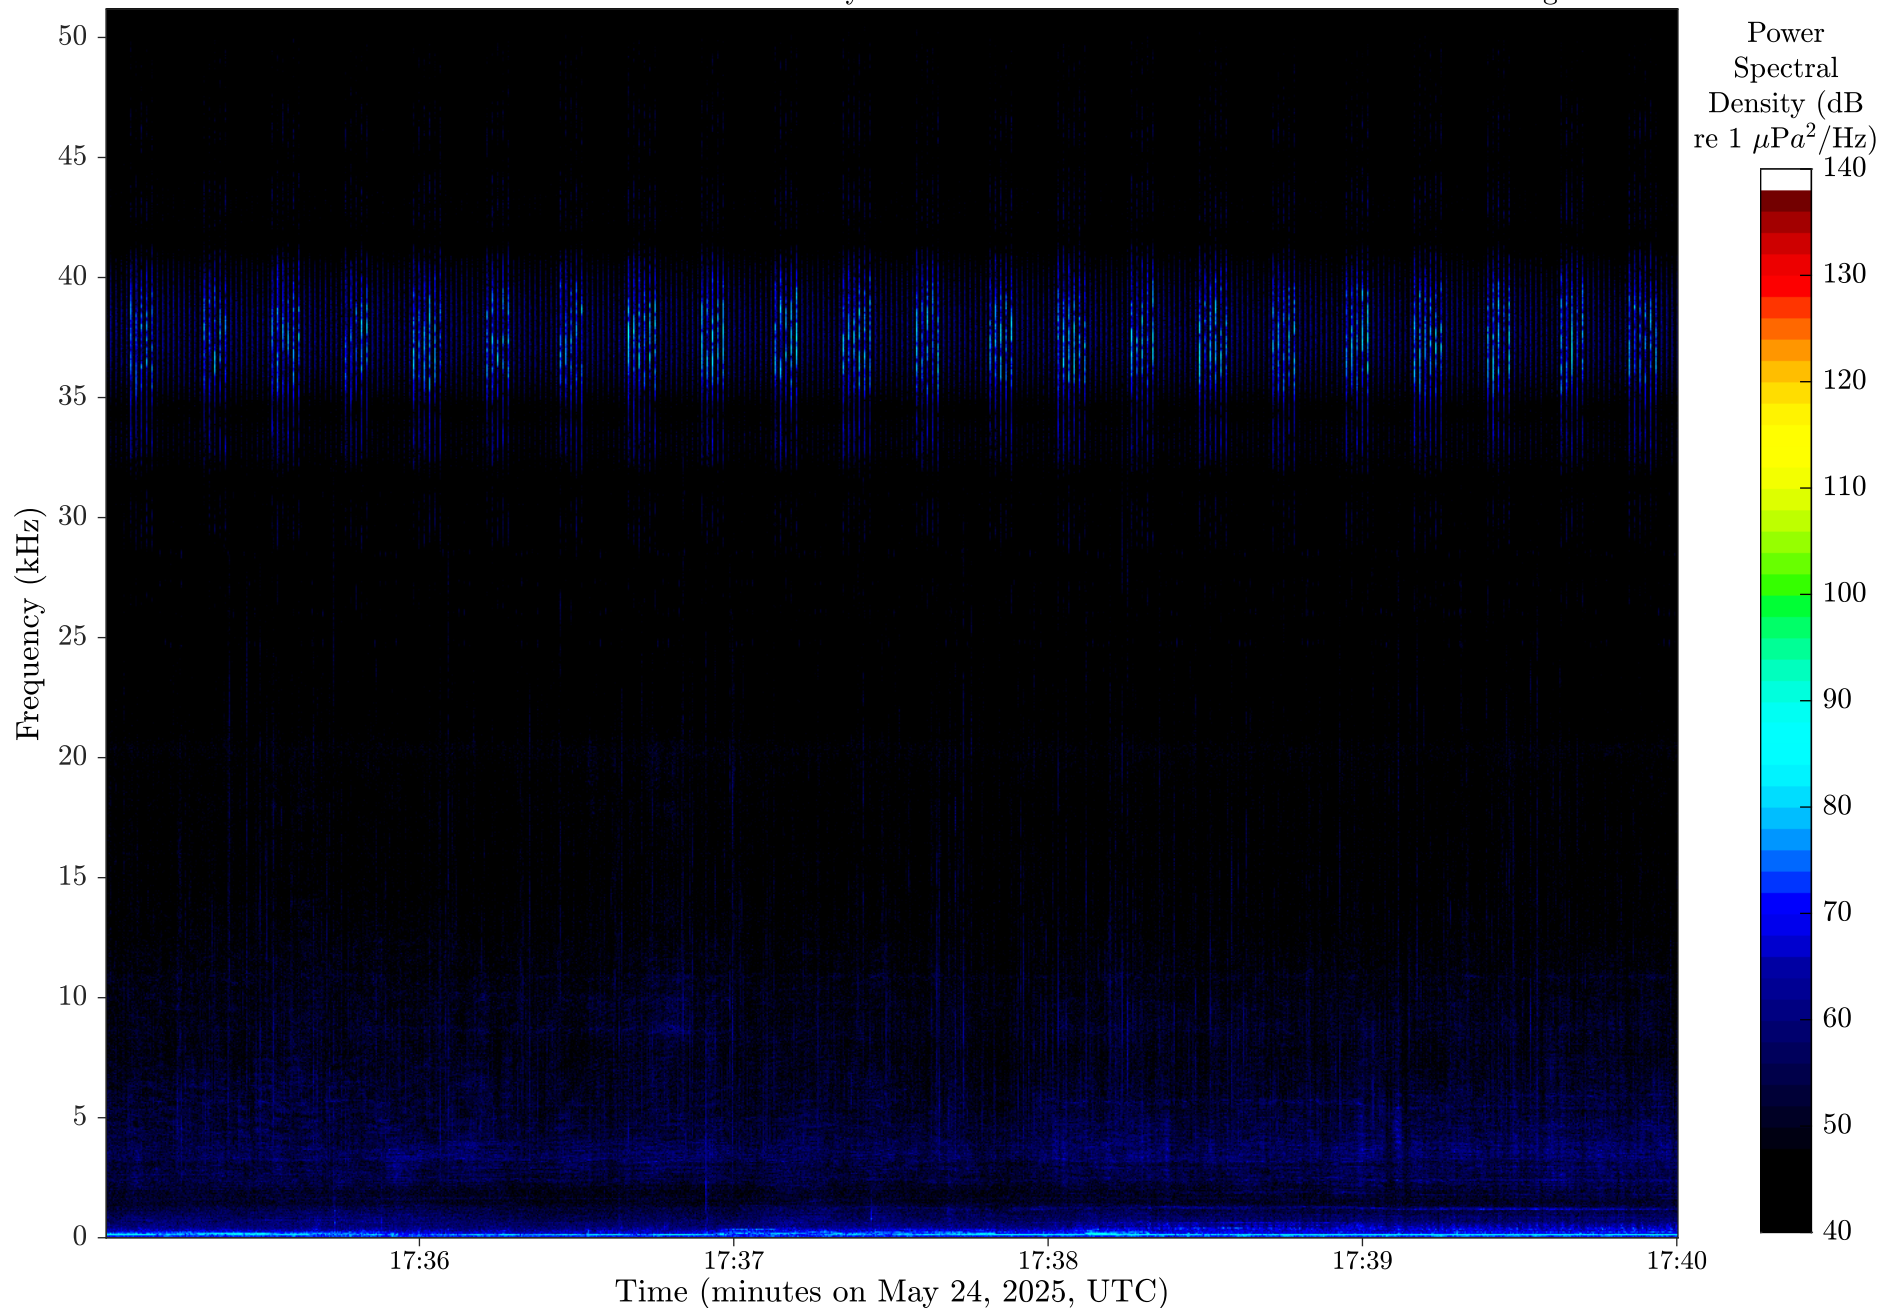


Comments: 30.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:05 UTC

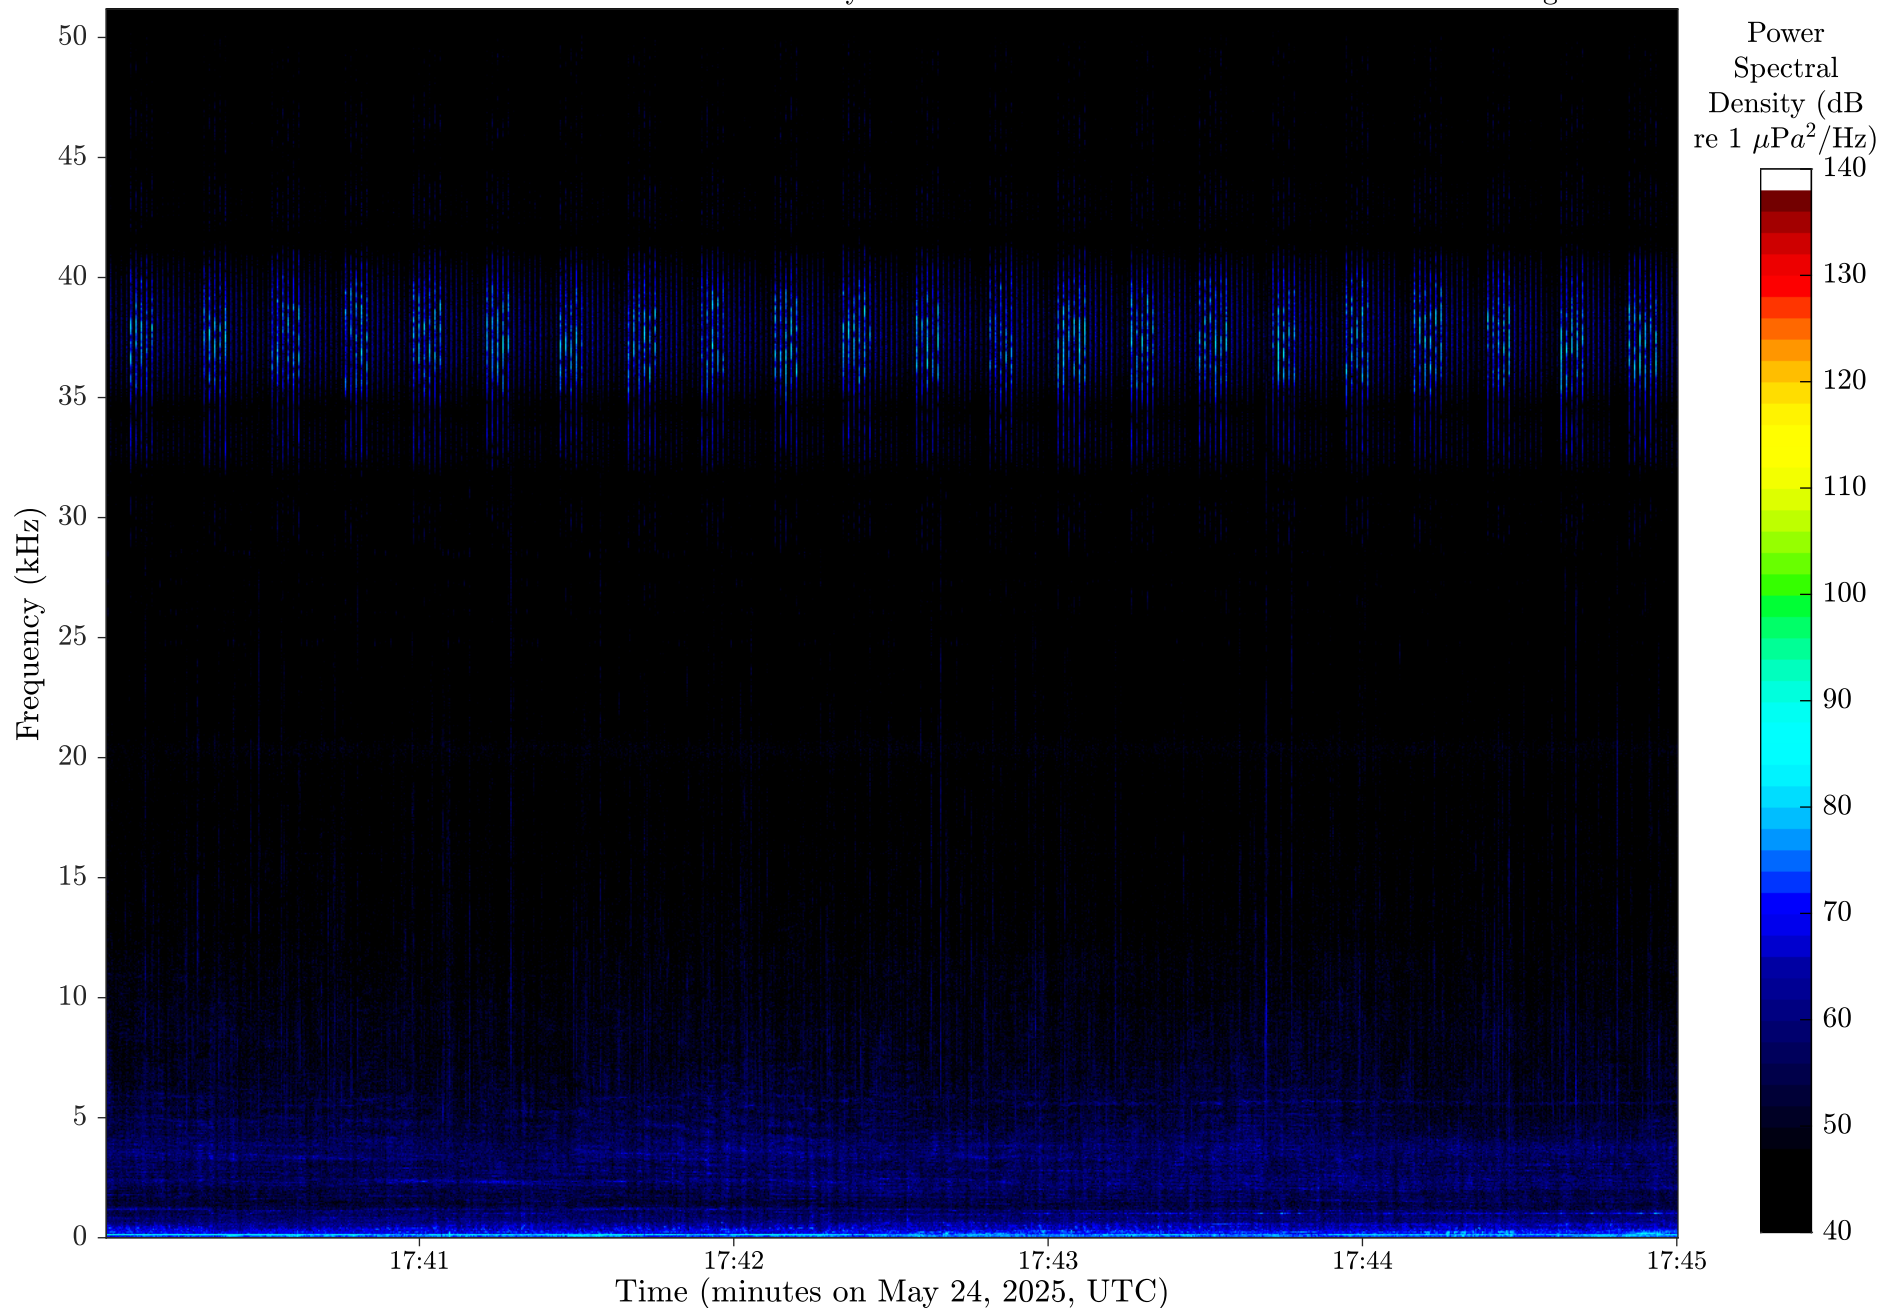


Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:13 UTC

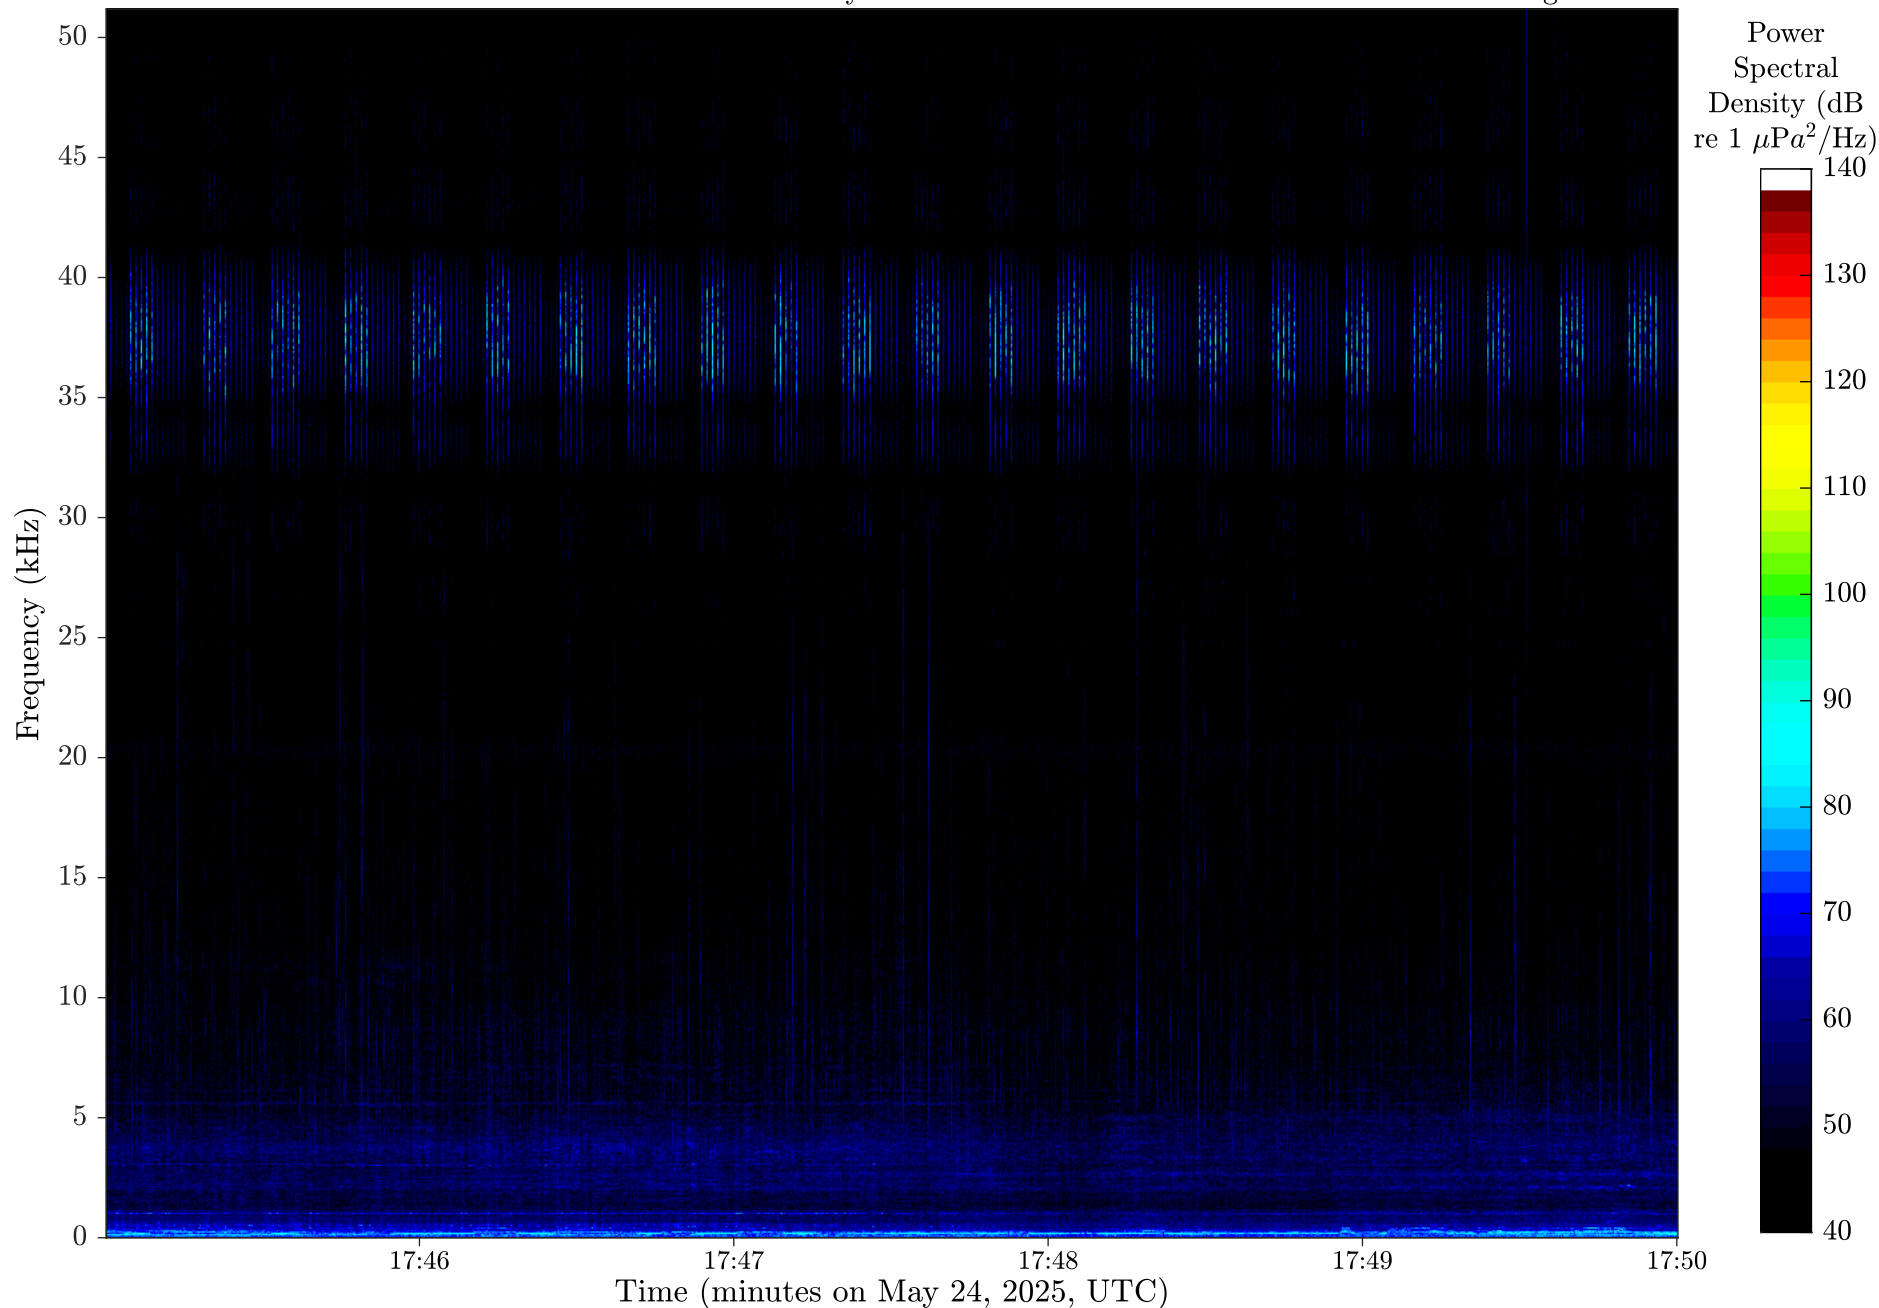


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:36:21 UTC

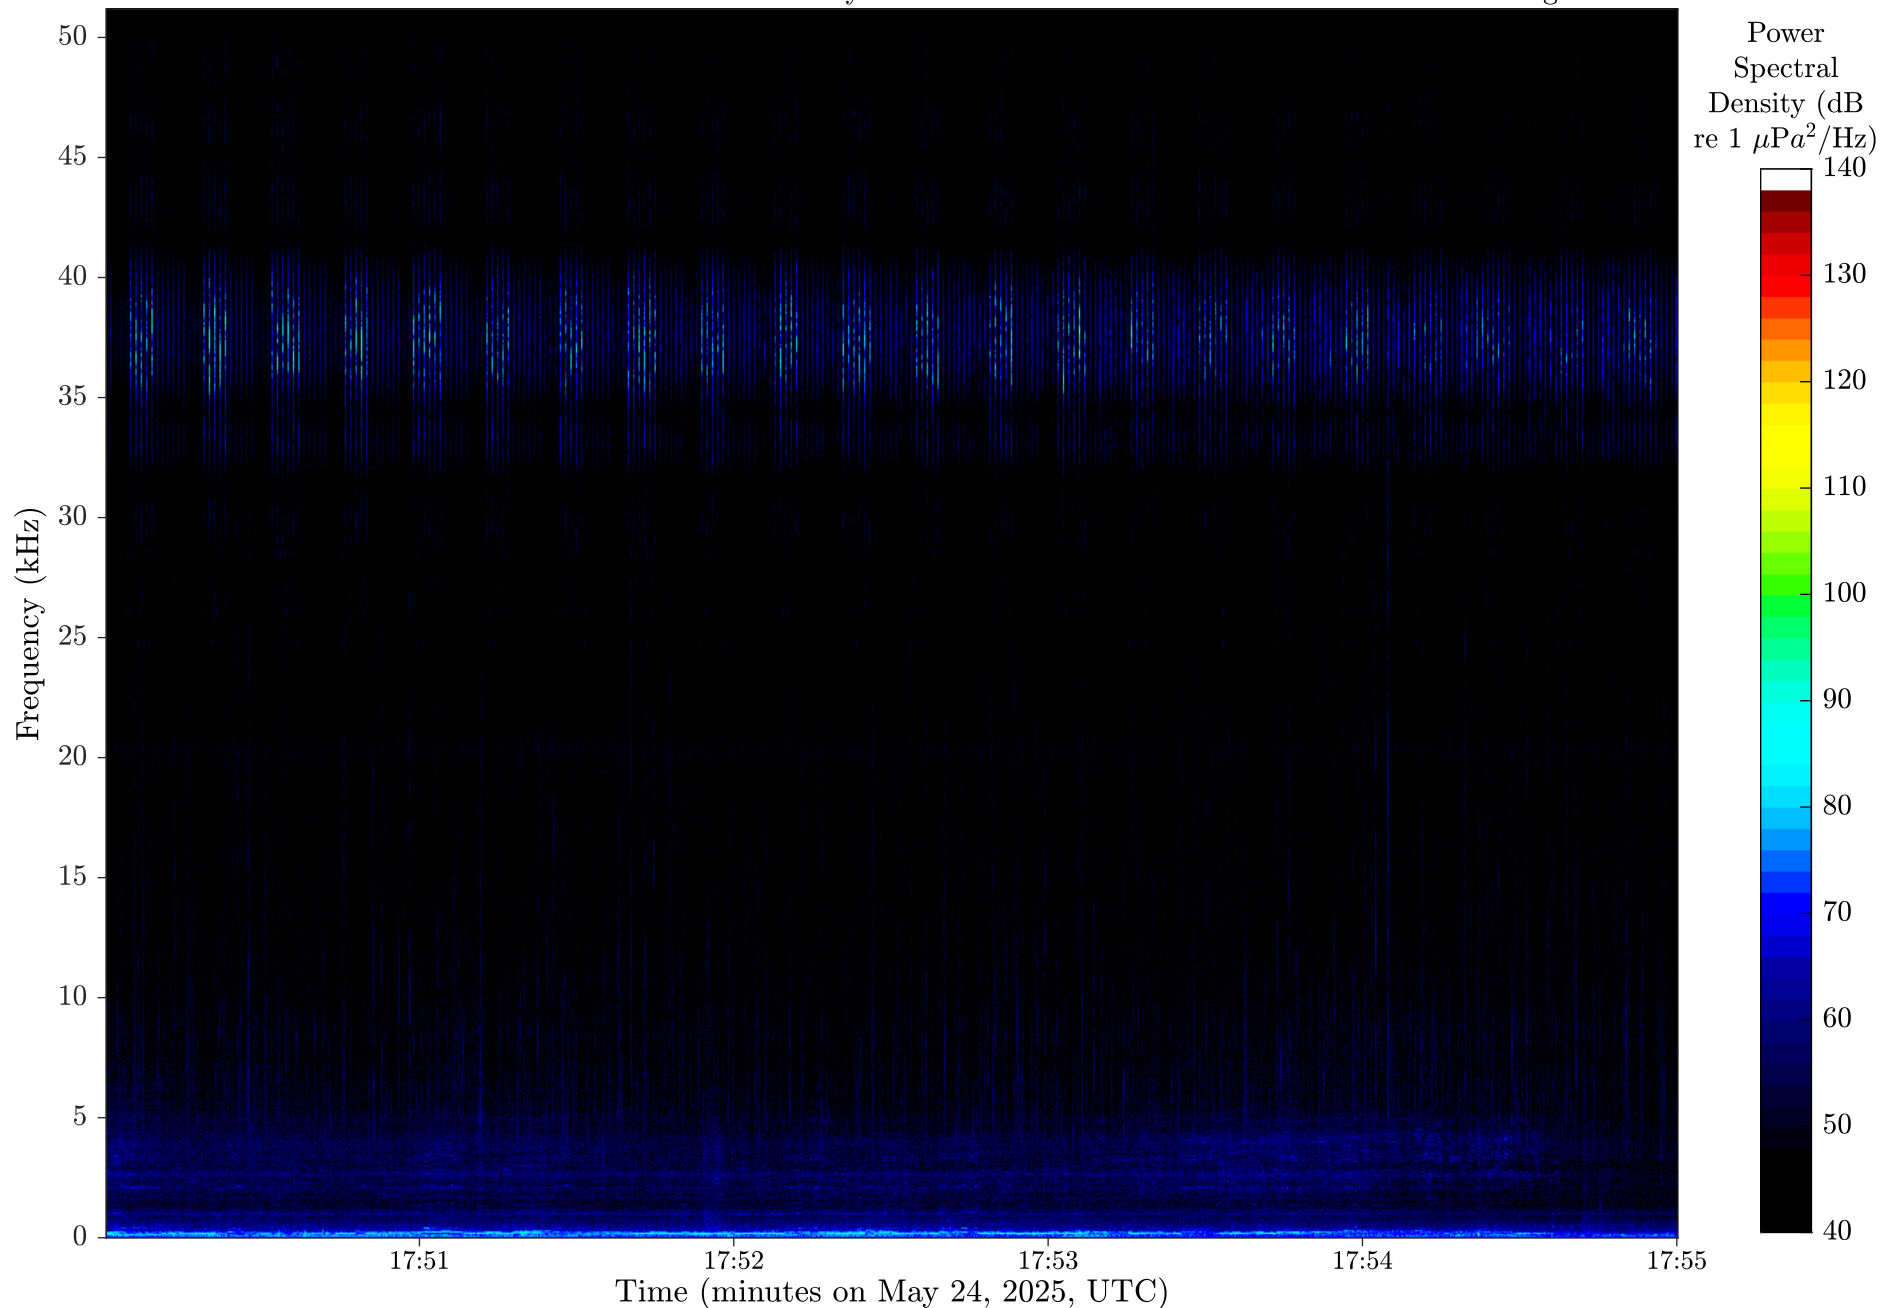

Comments: 32.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:36:29 UTC

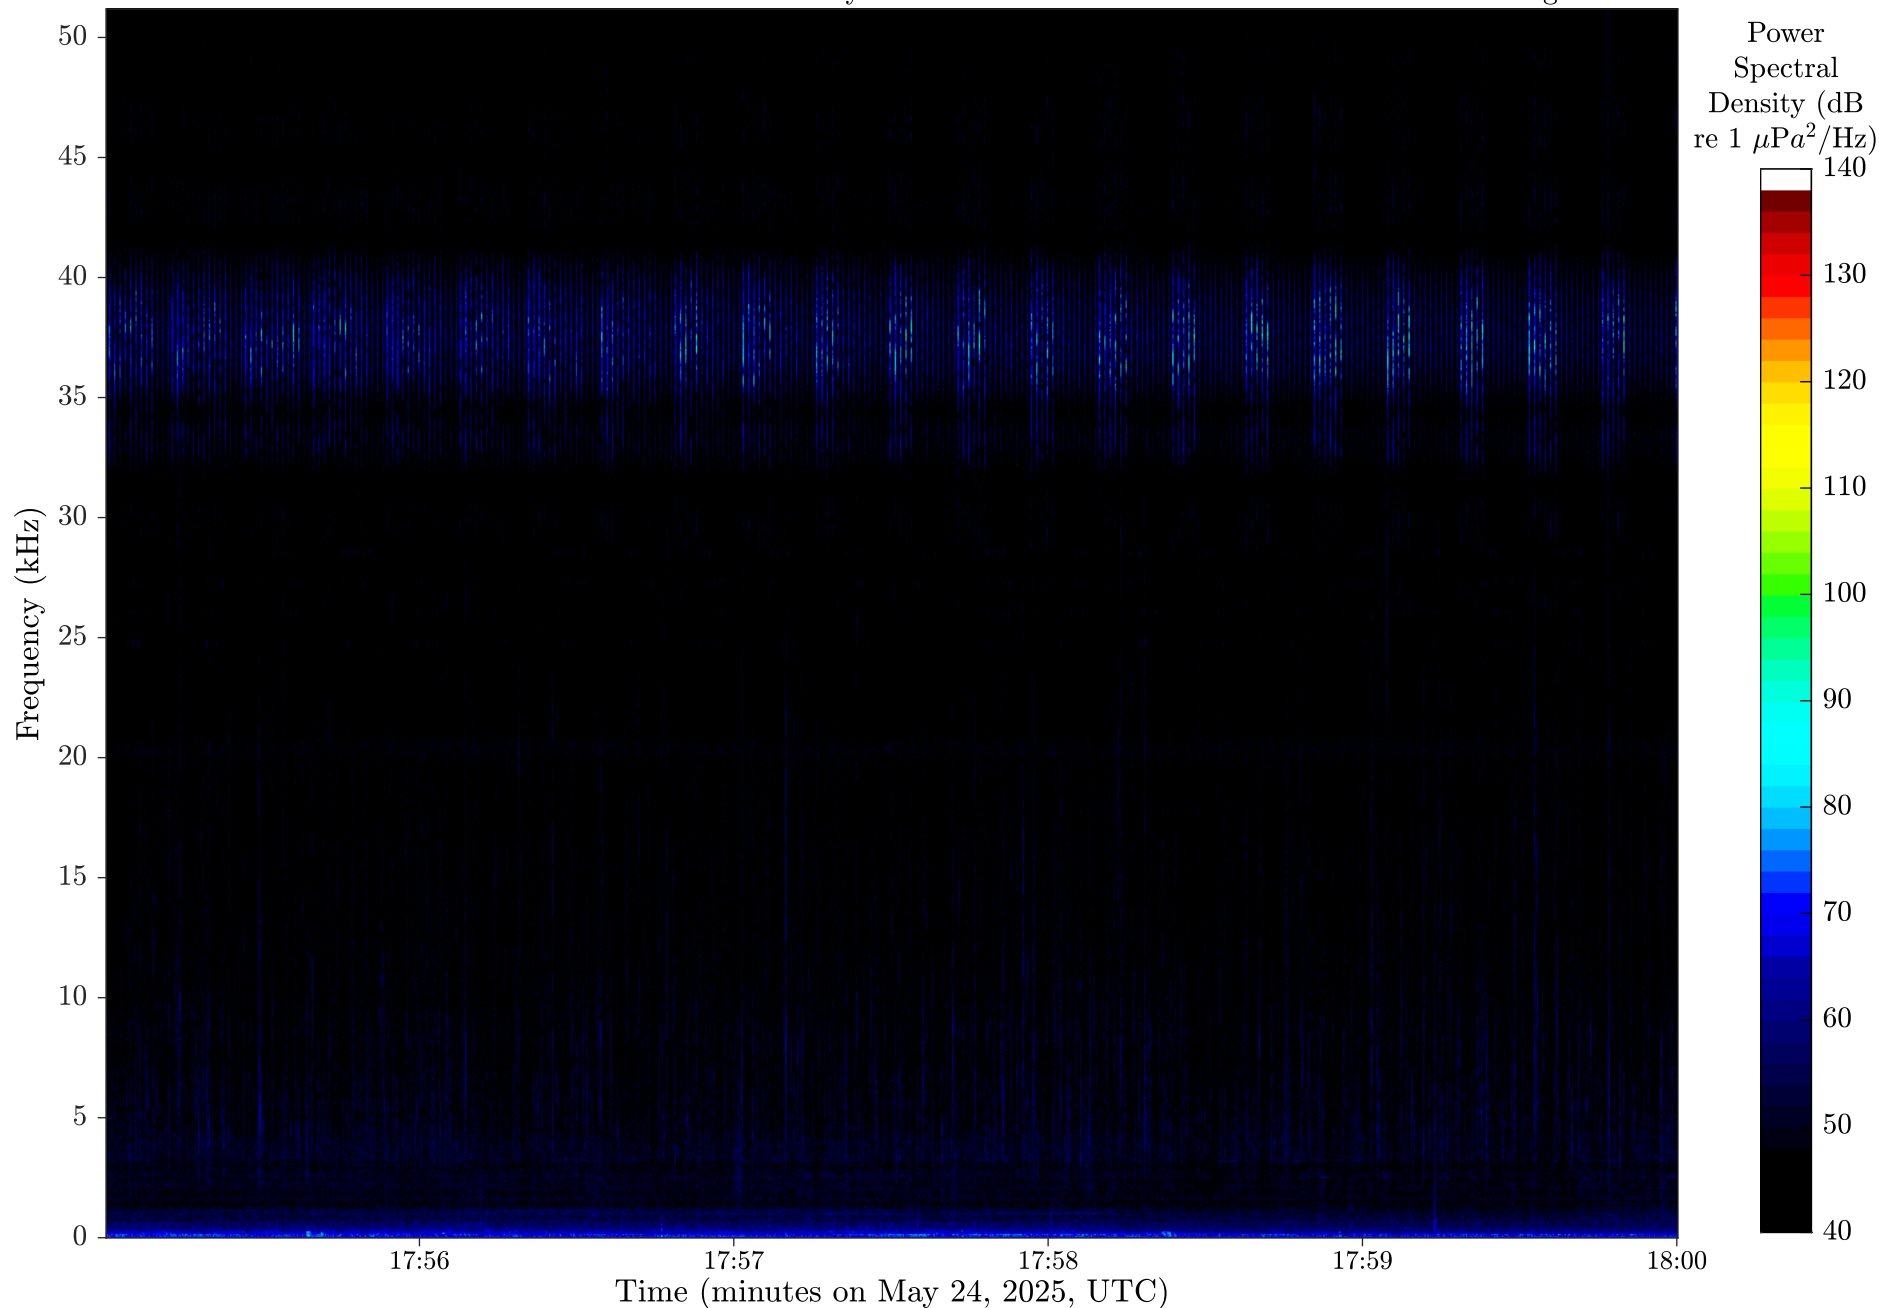

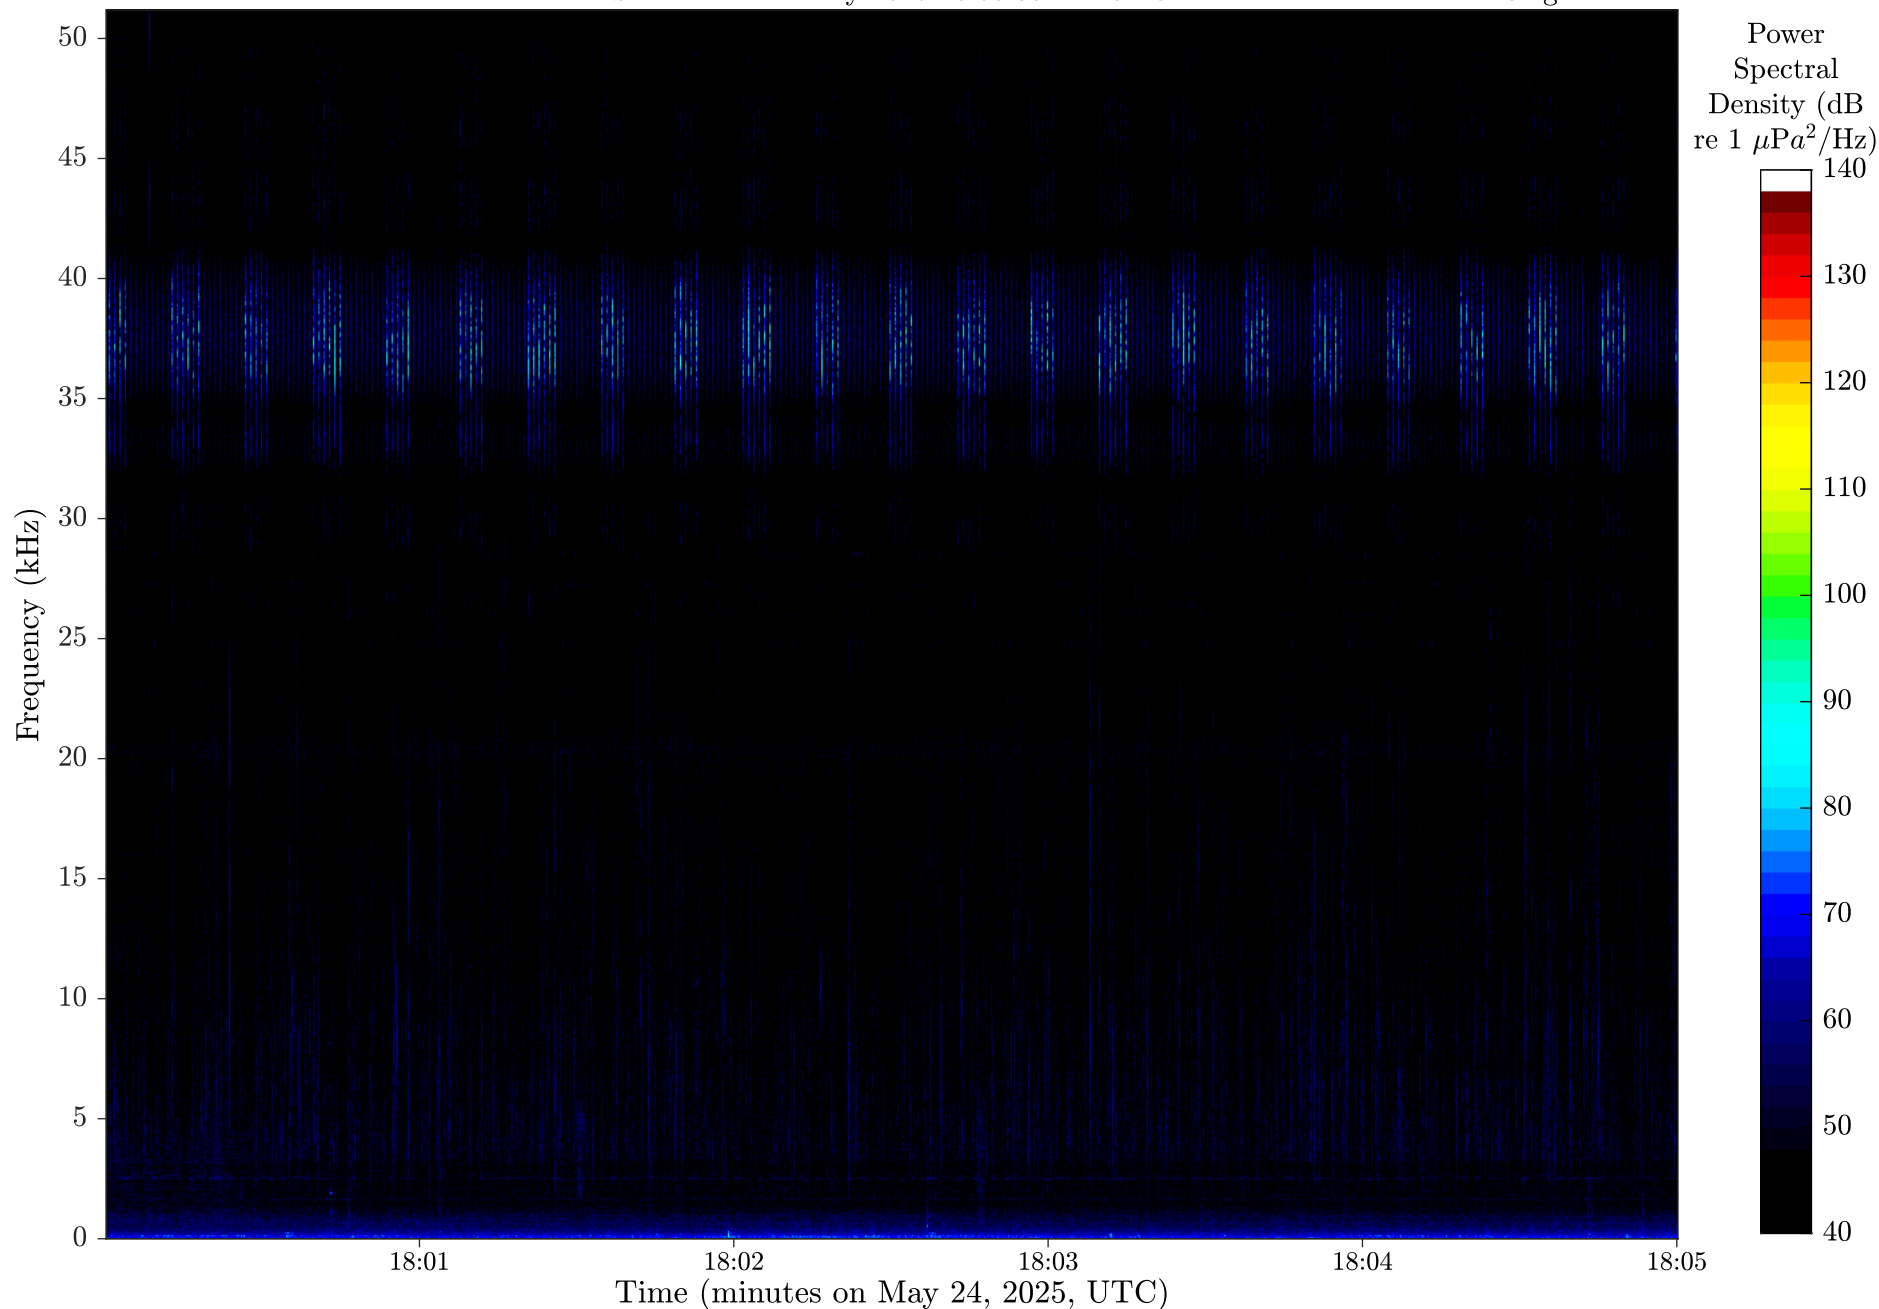


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:45 UTC

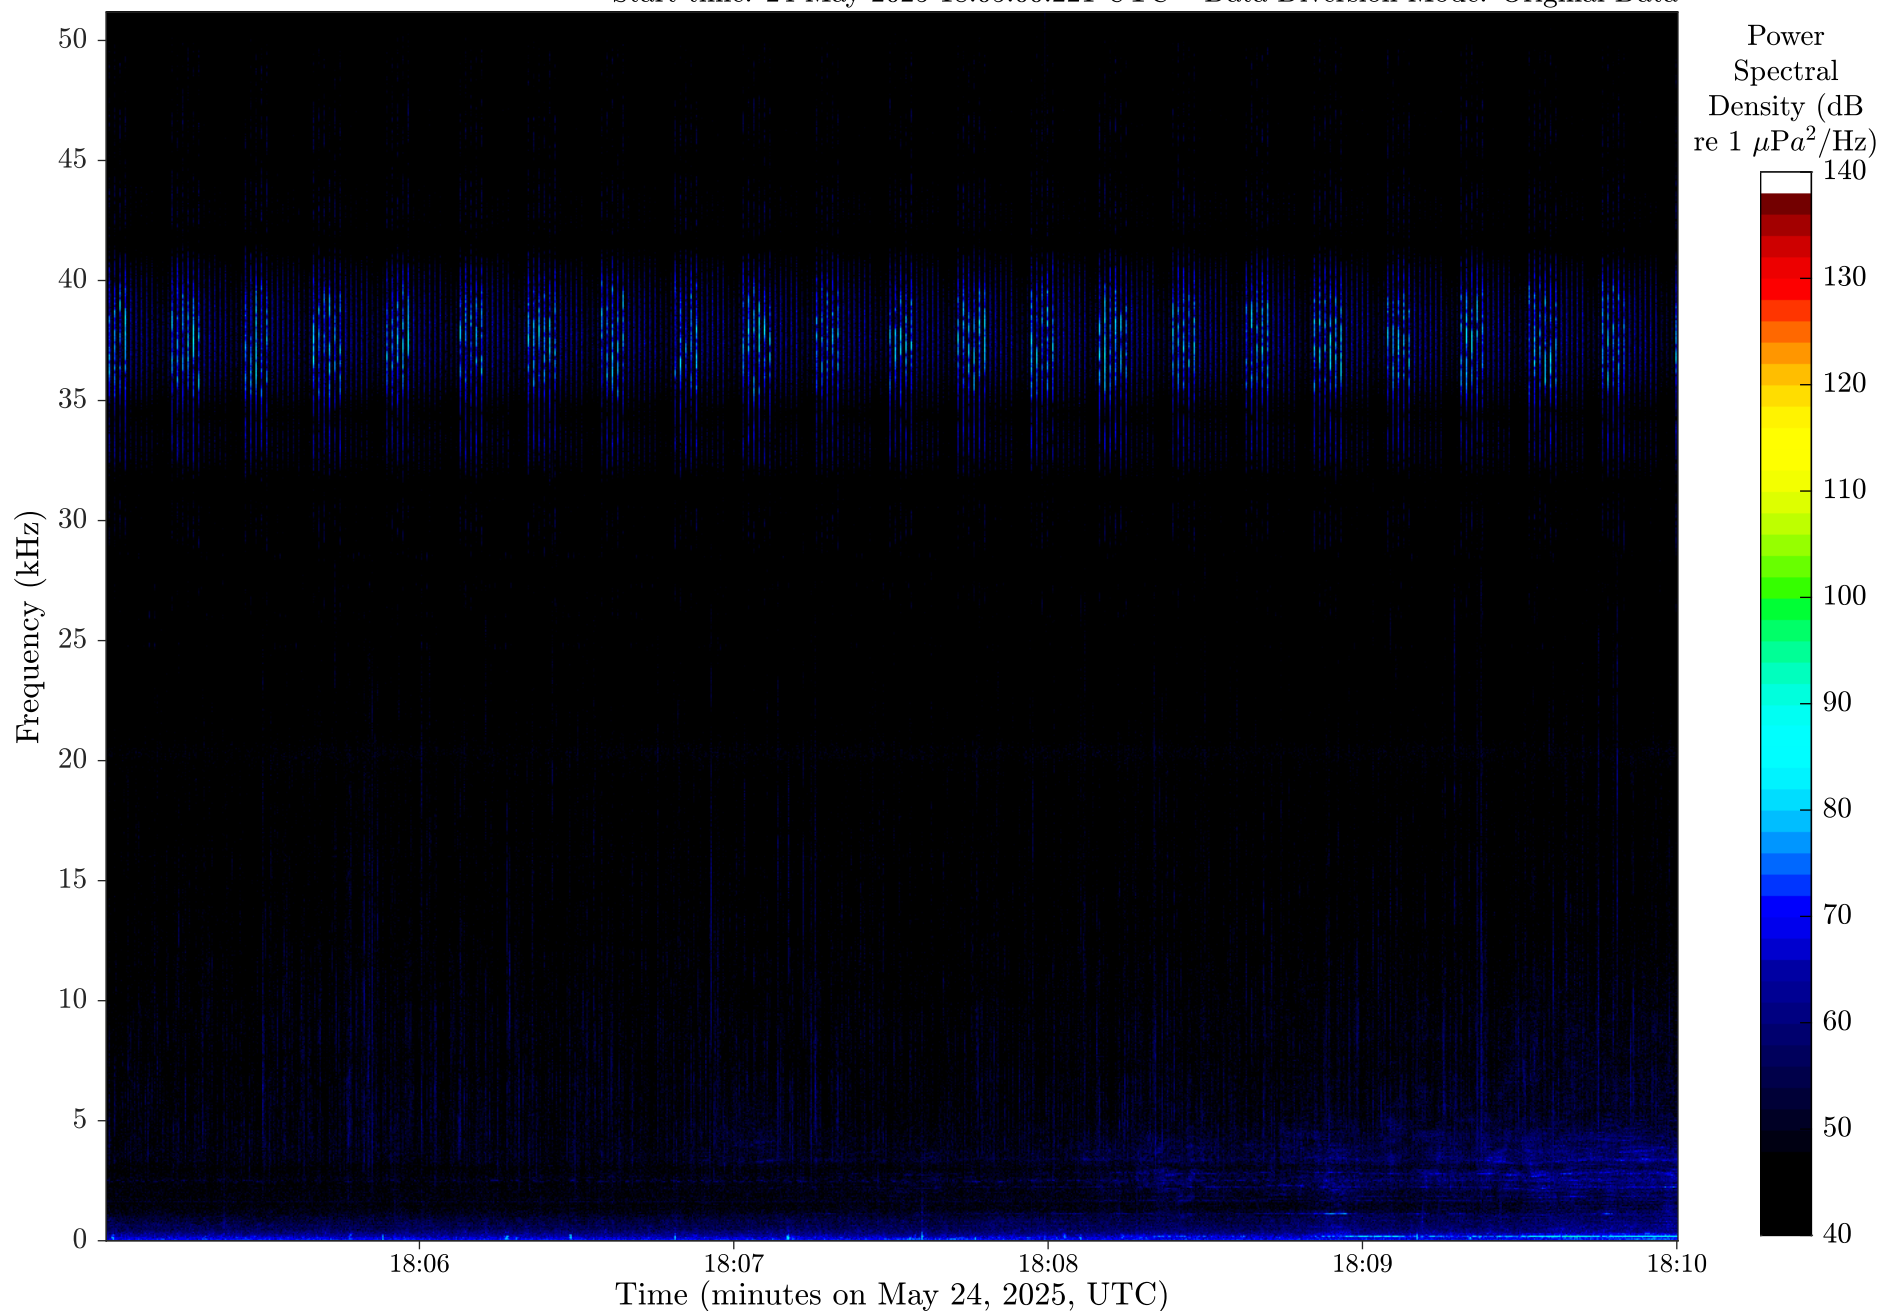


Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:54 UTC

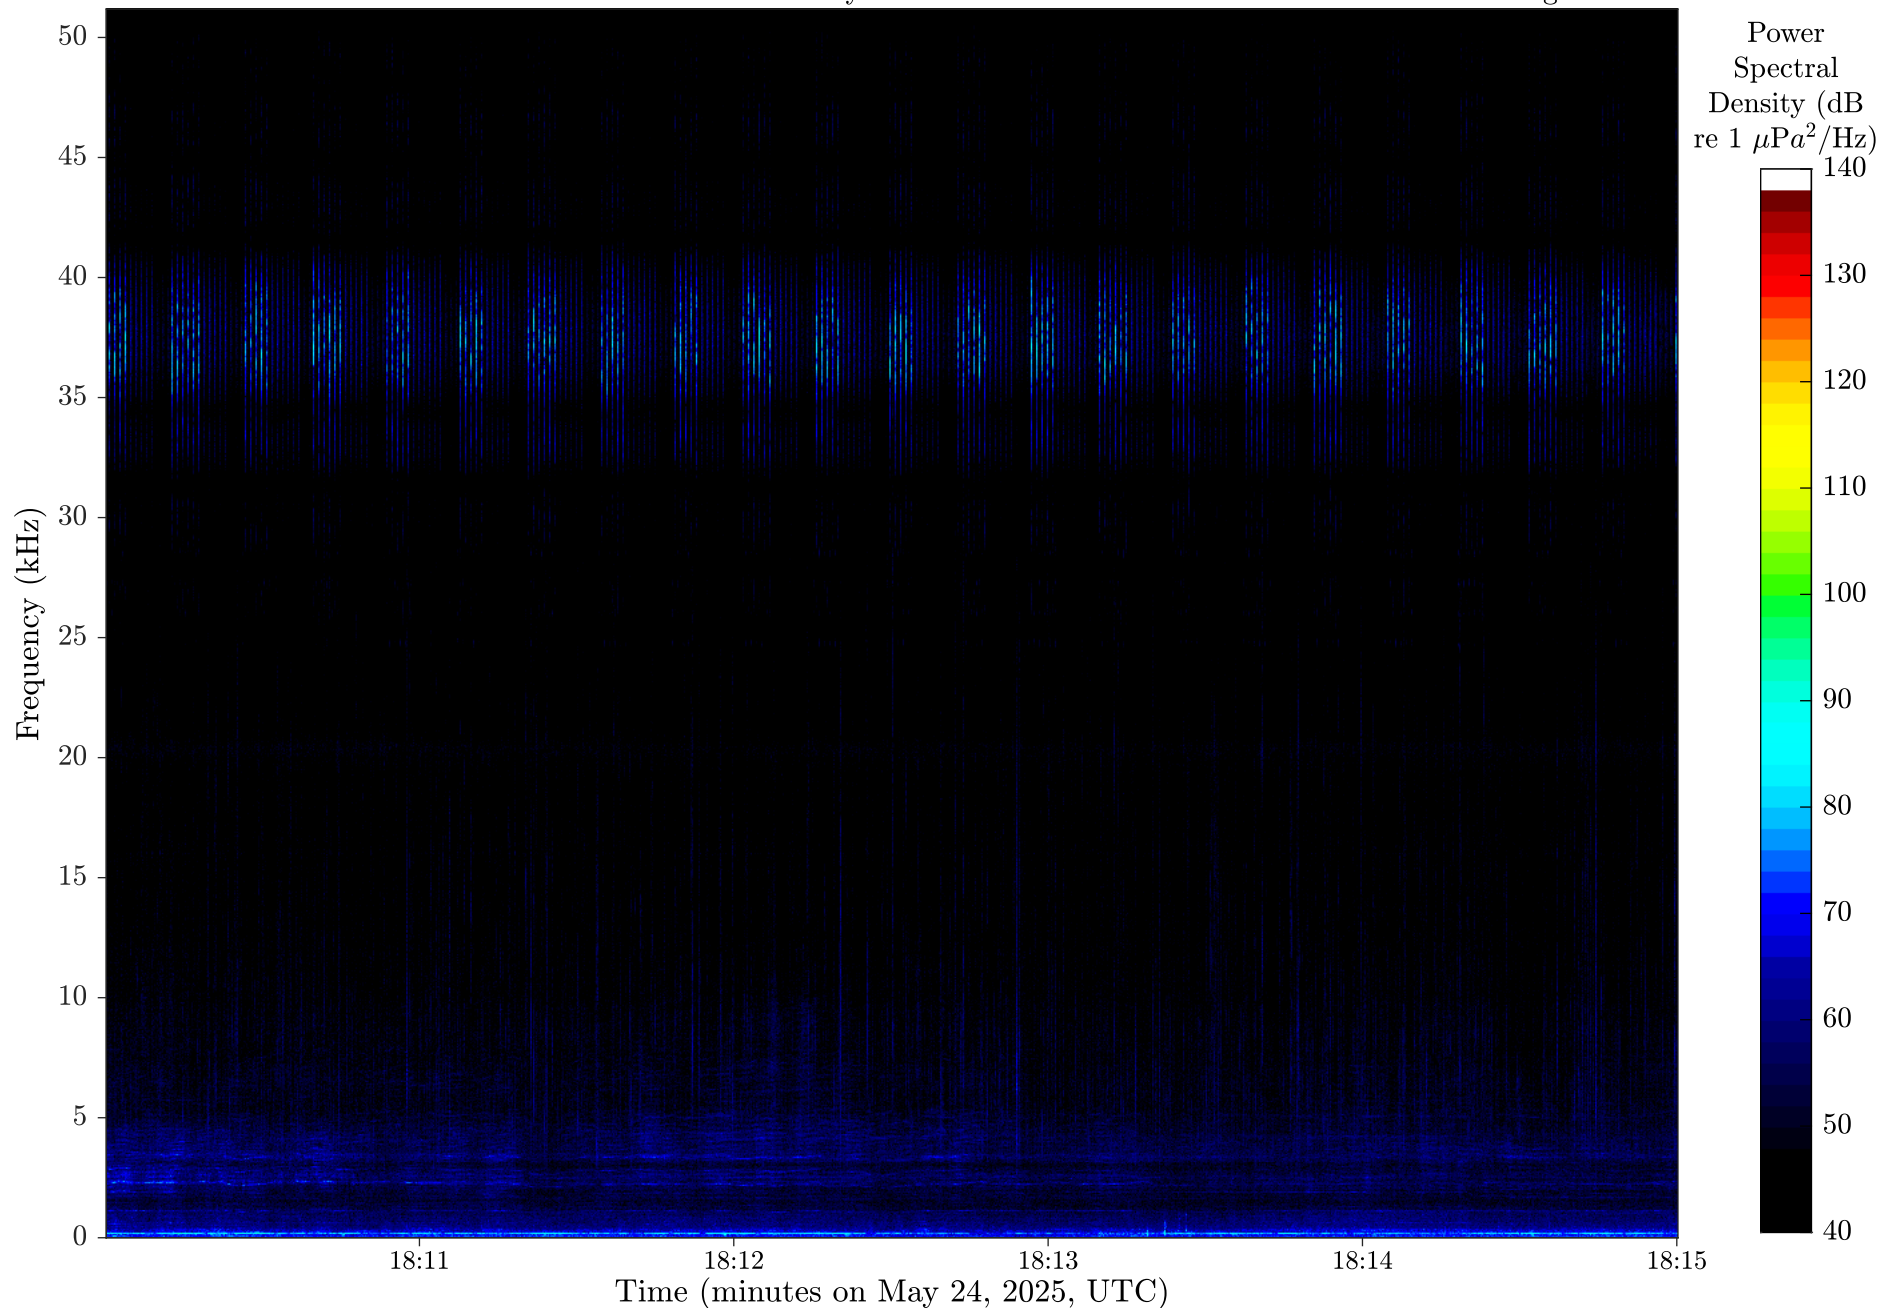


Comments: 32.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:01 UTC

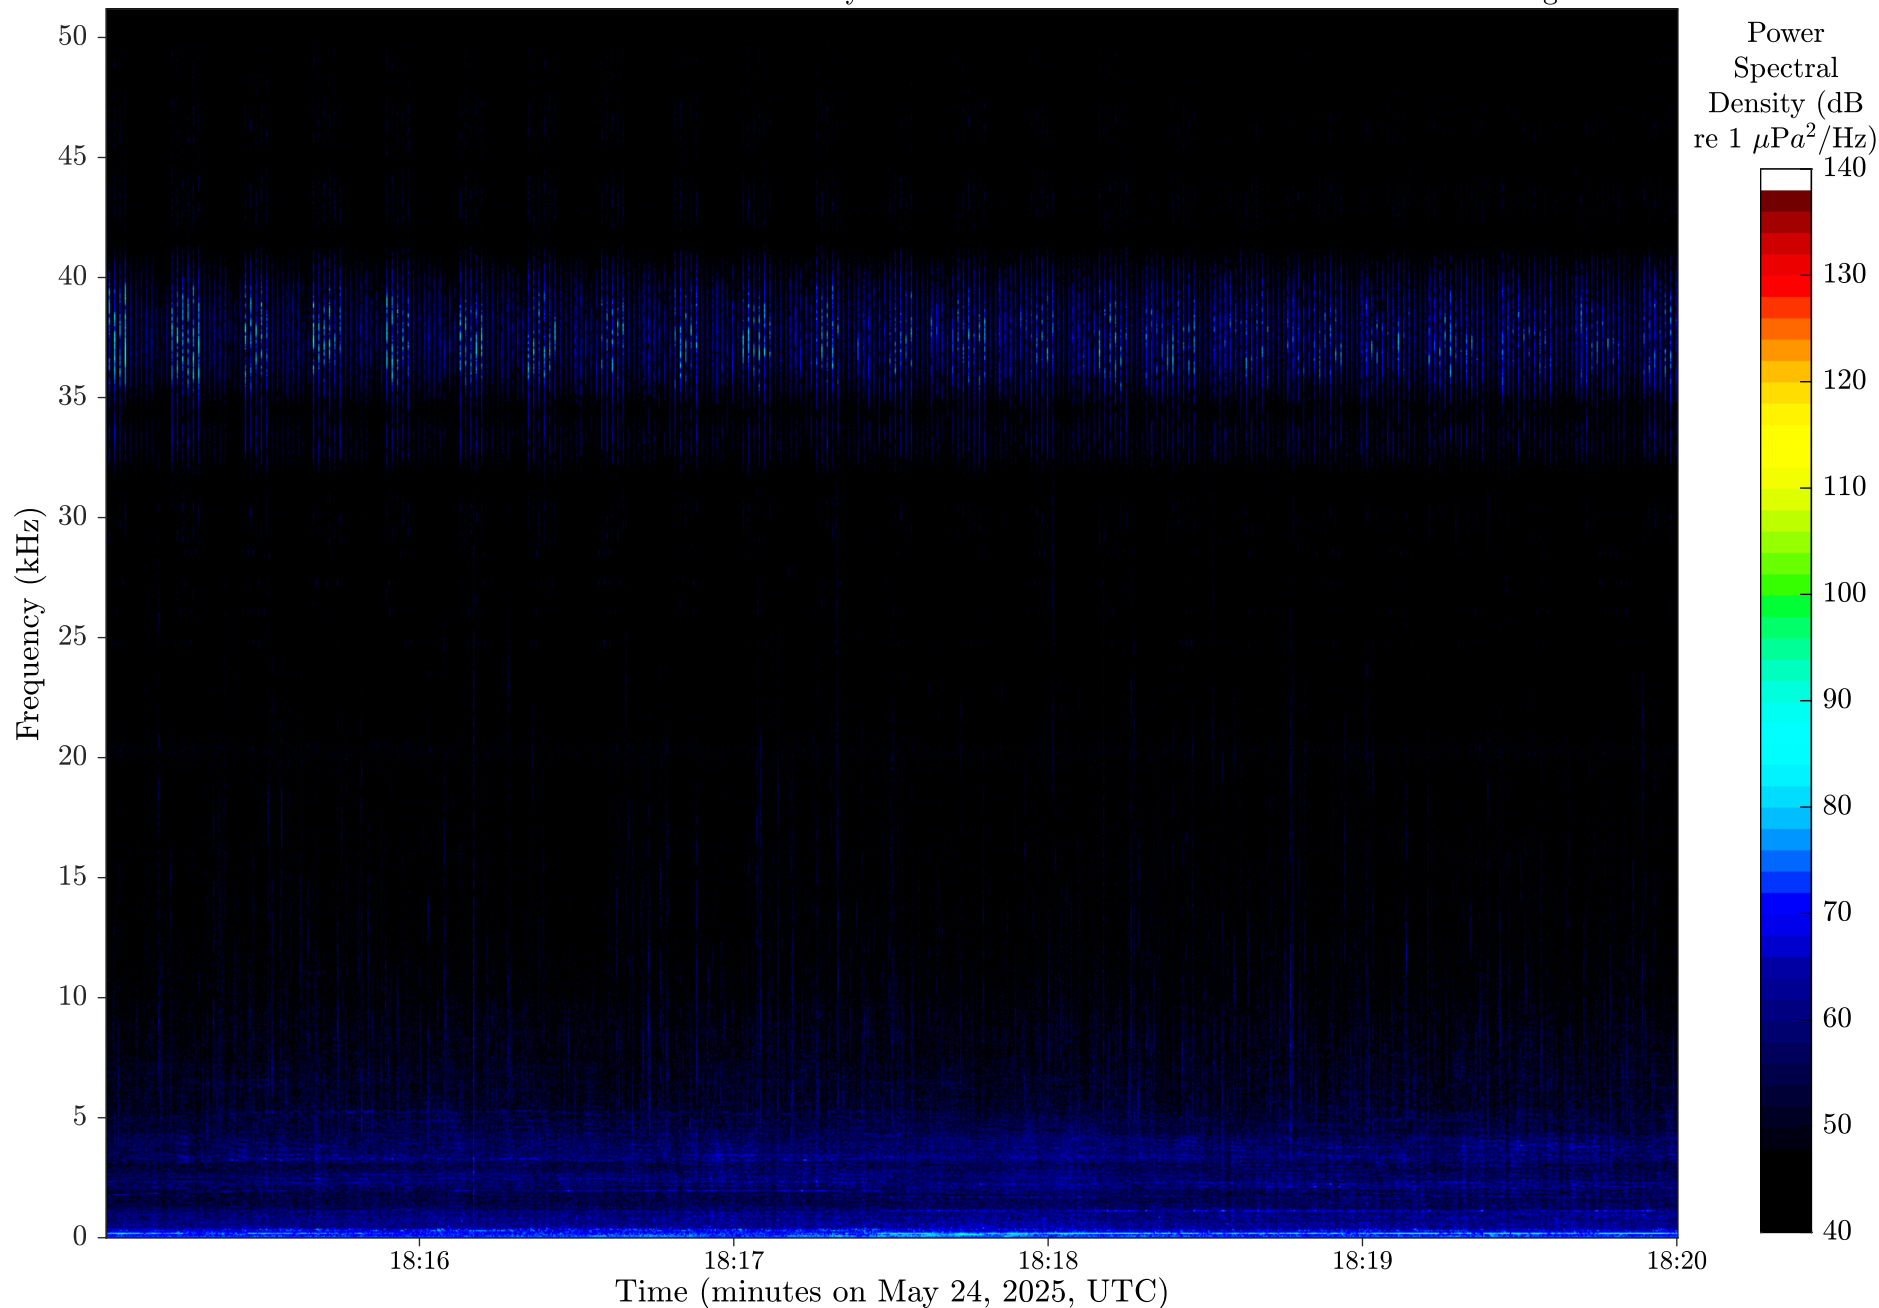


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:09 UTC

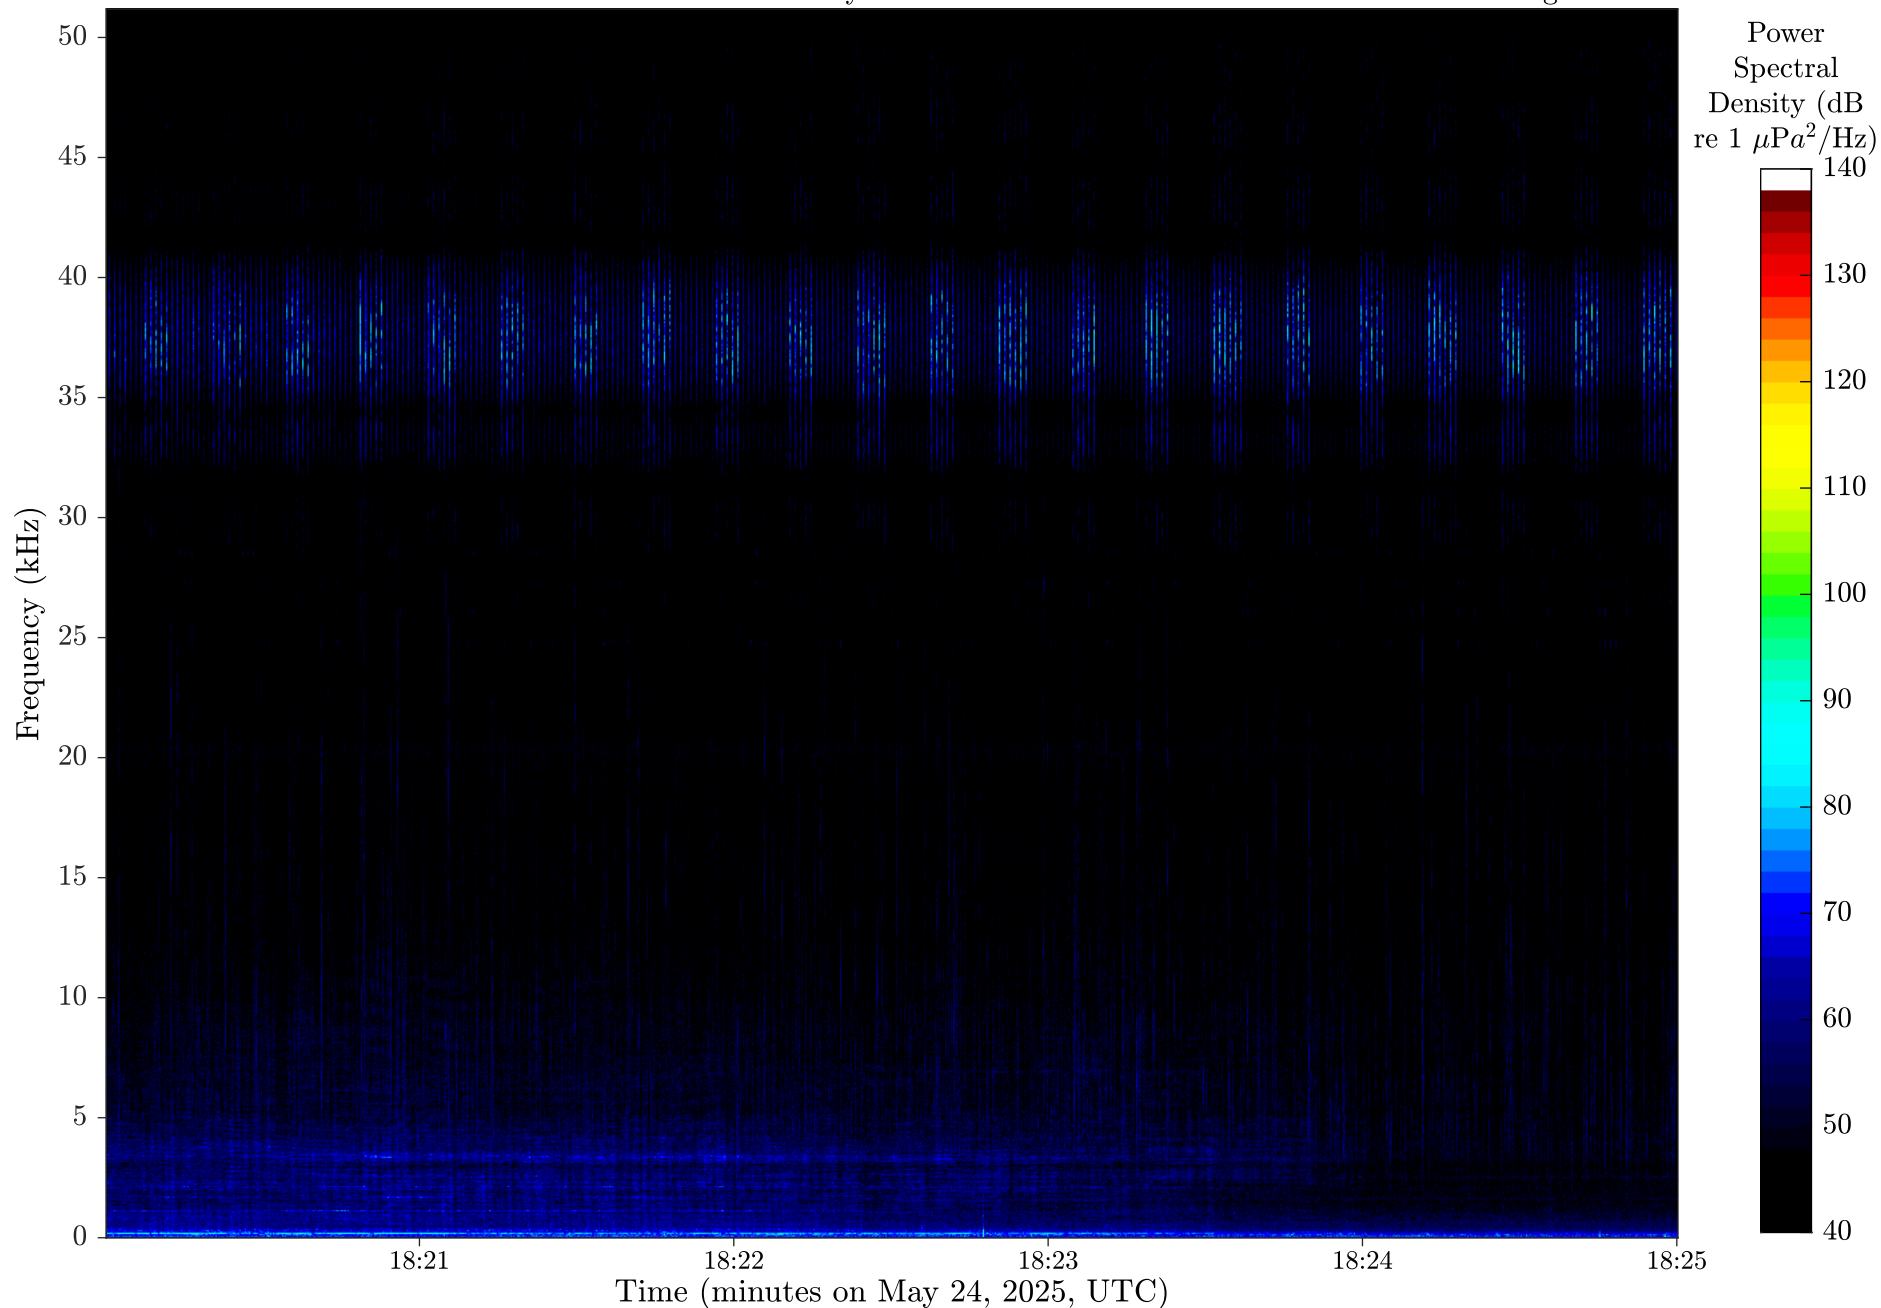


Comments: 31.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:17 UTC

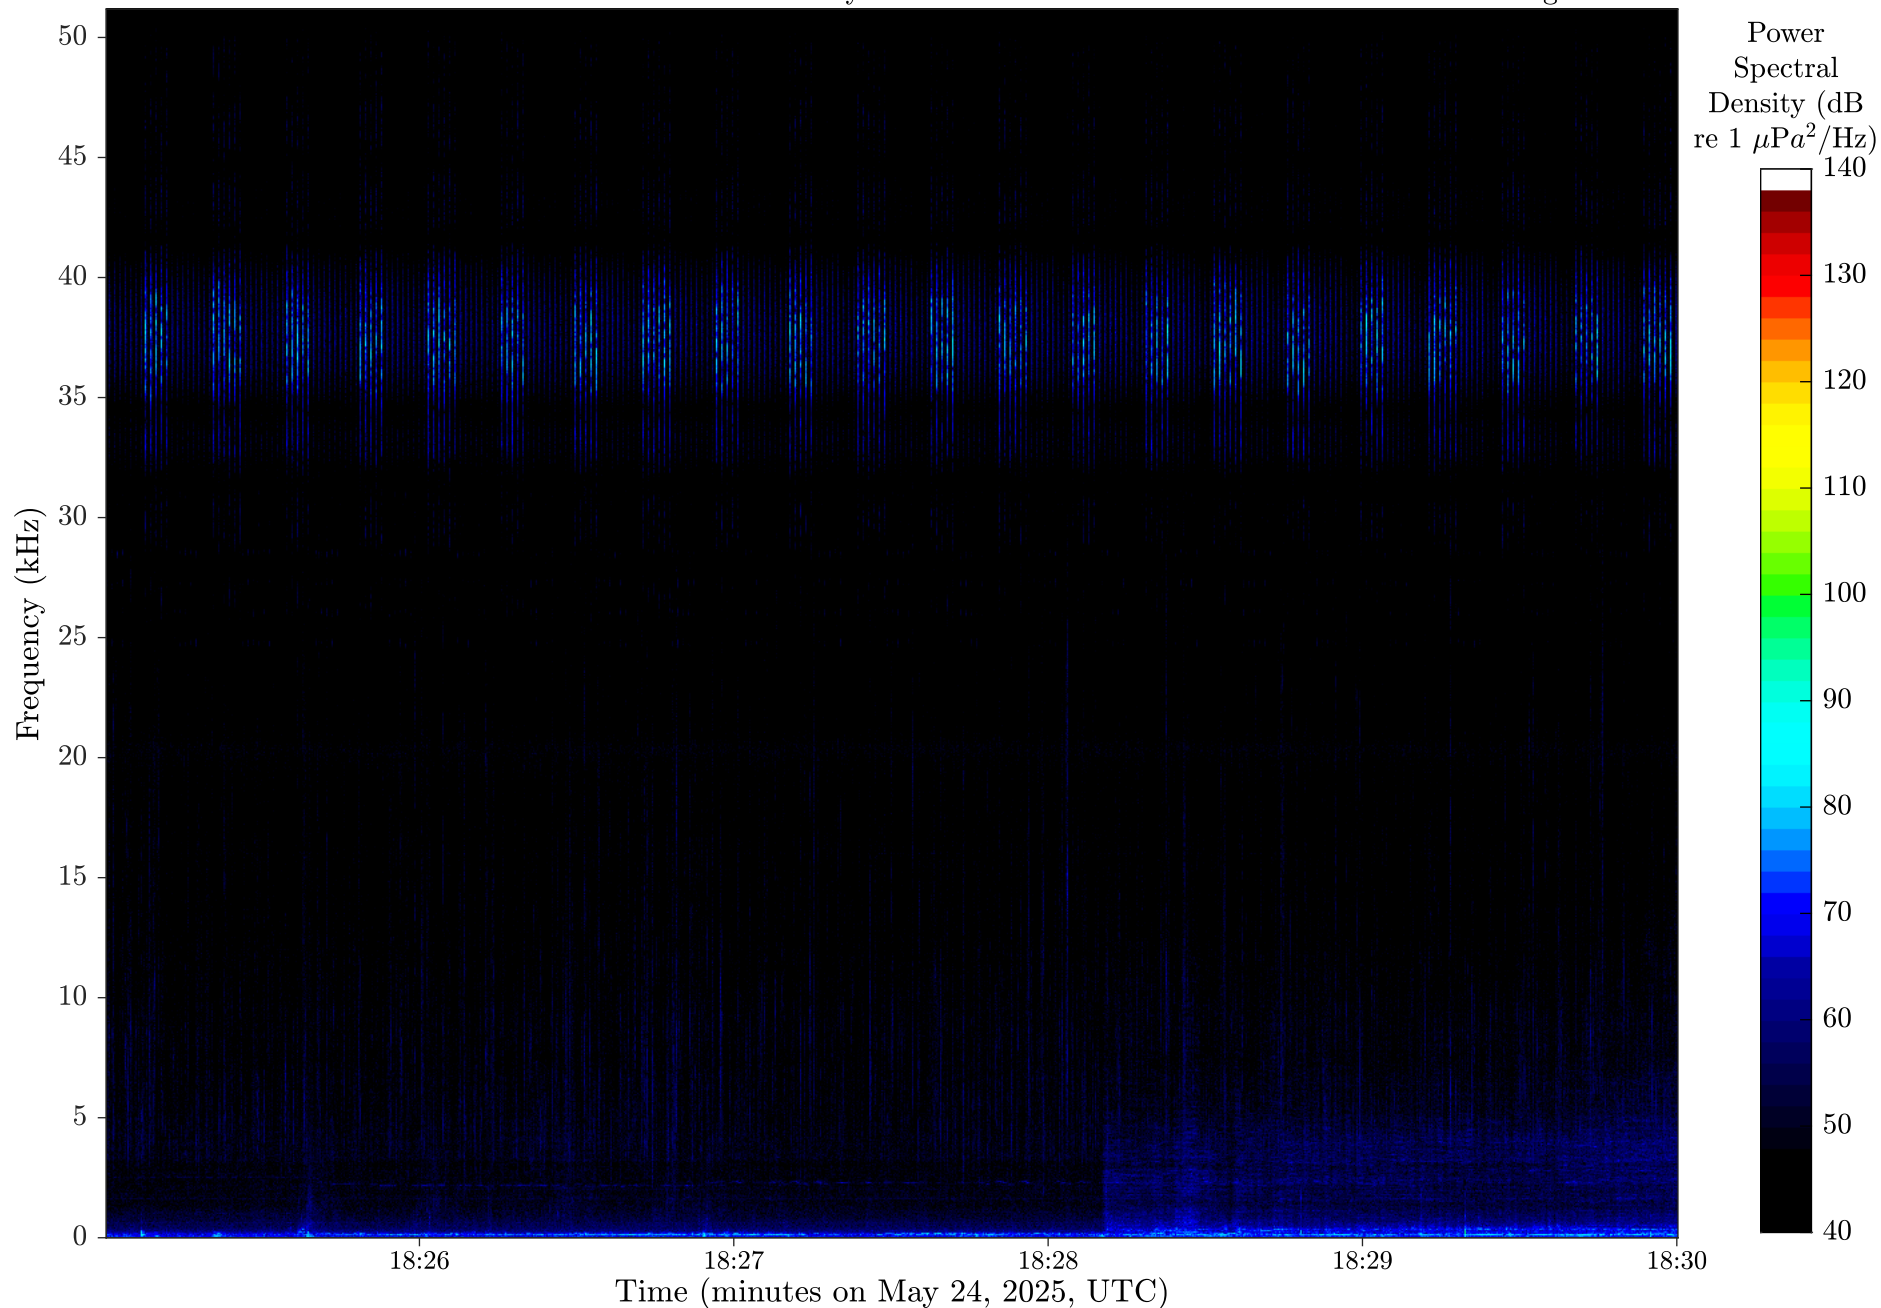


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:25 UTC

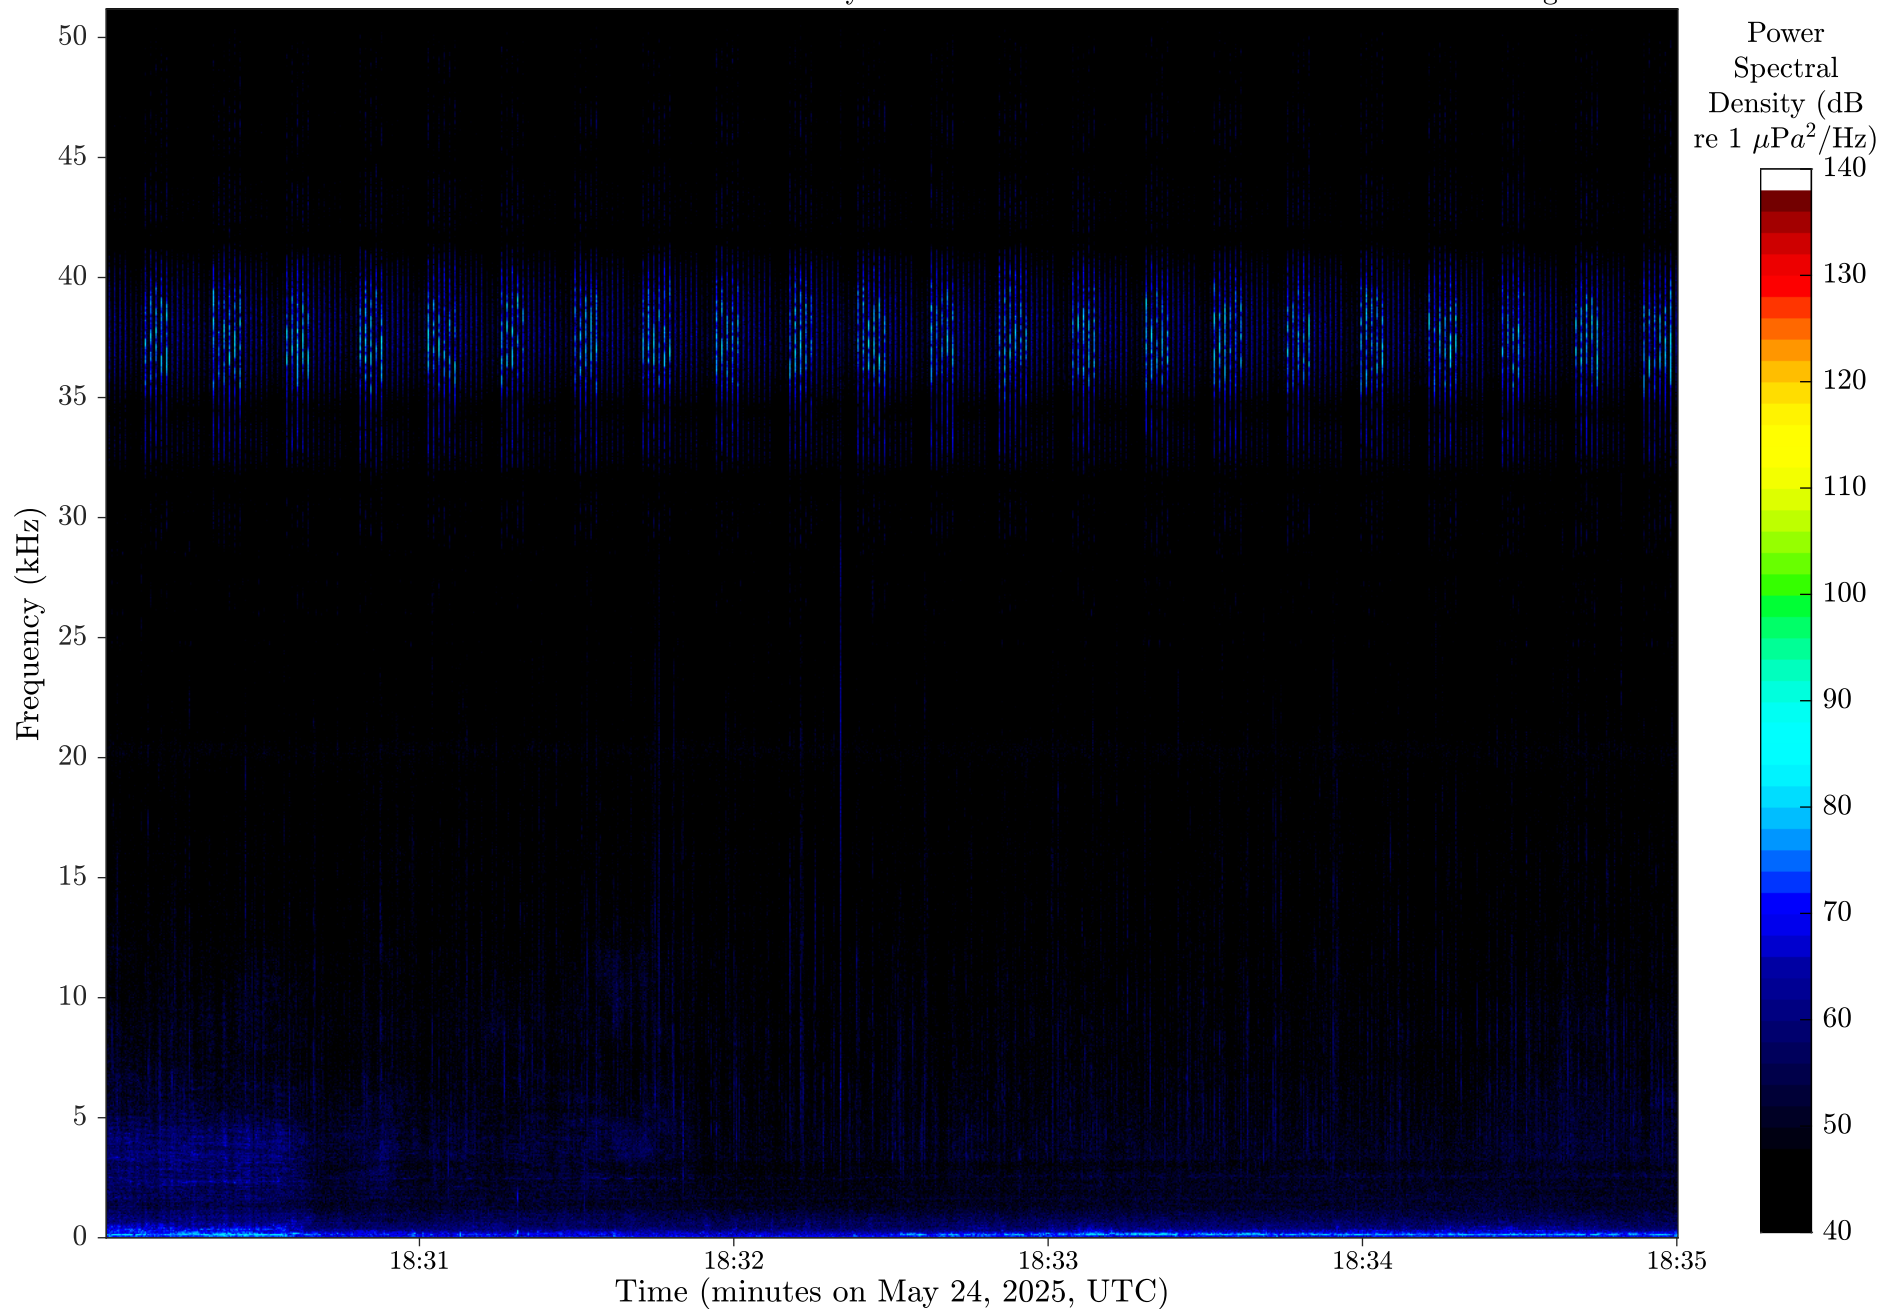


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:33 UTC

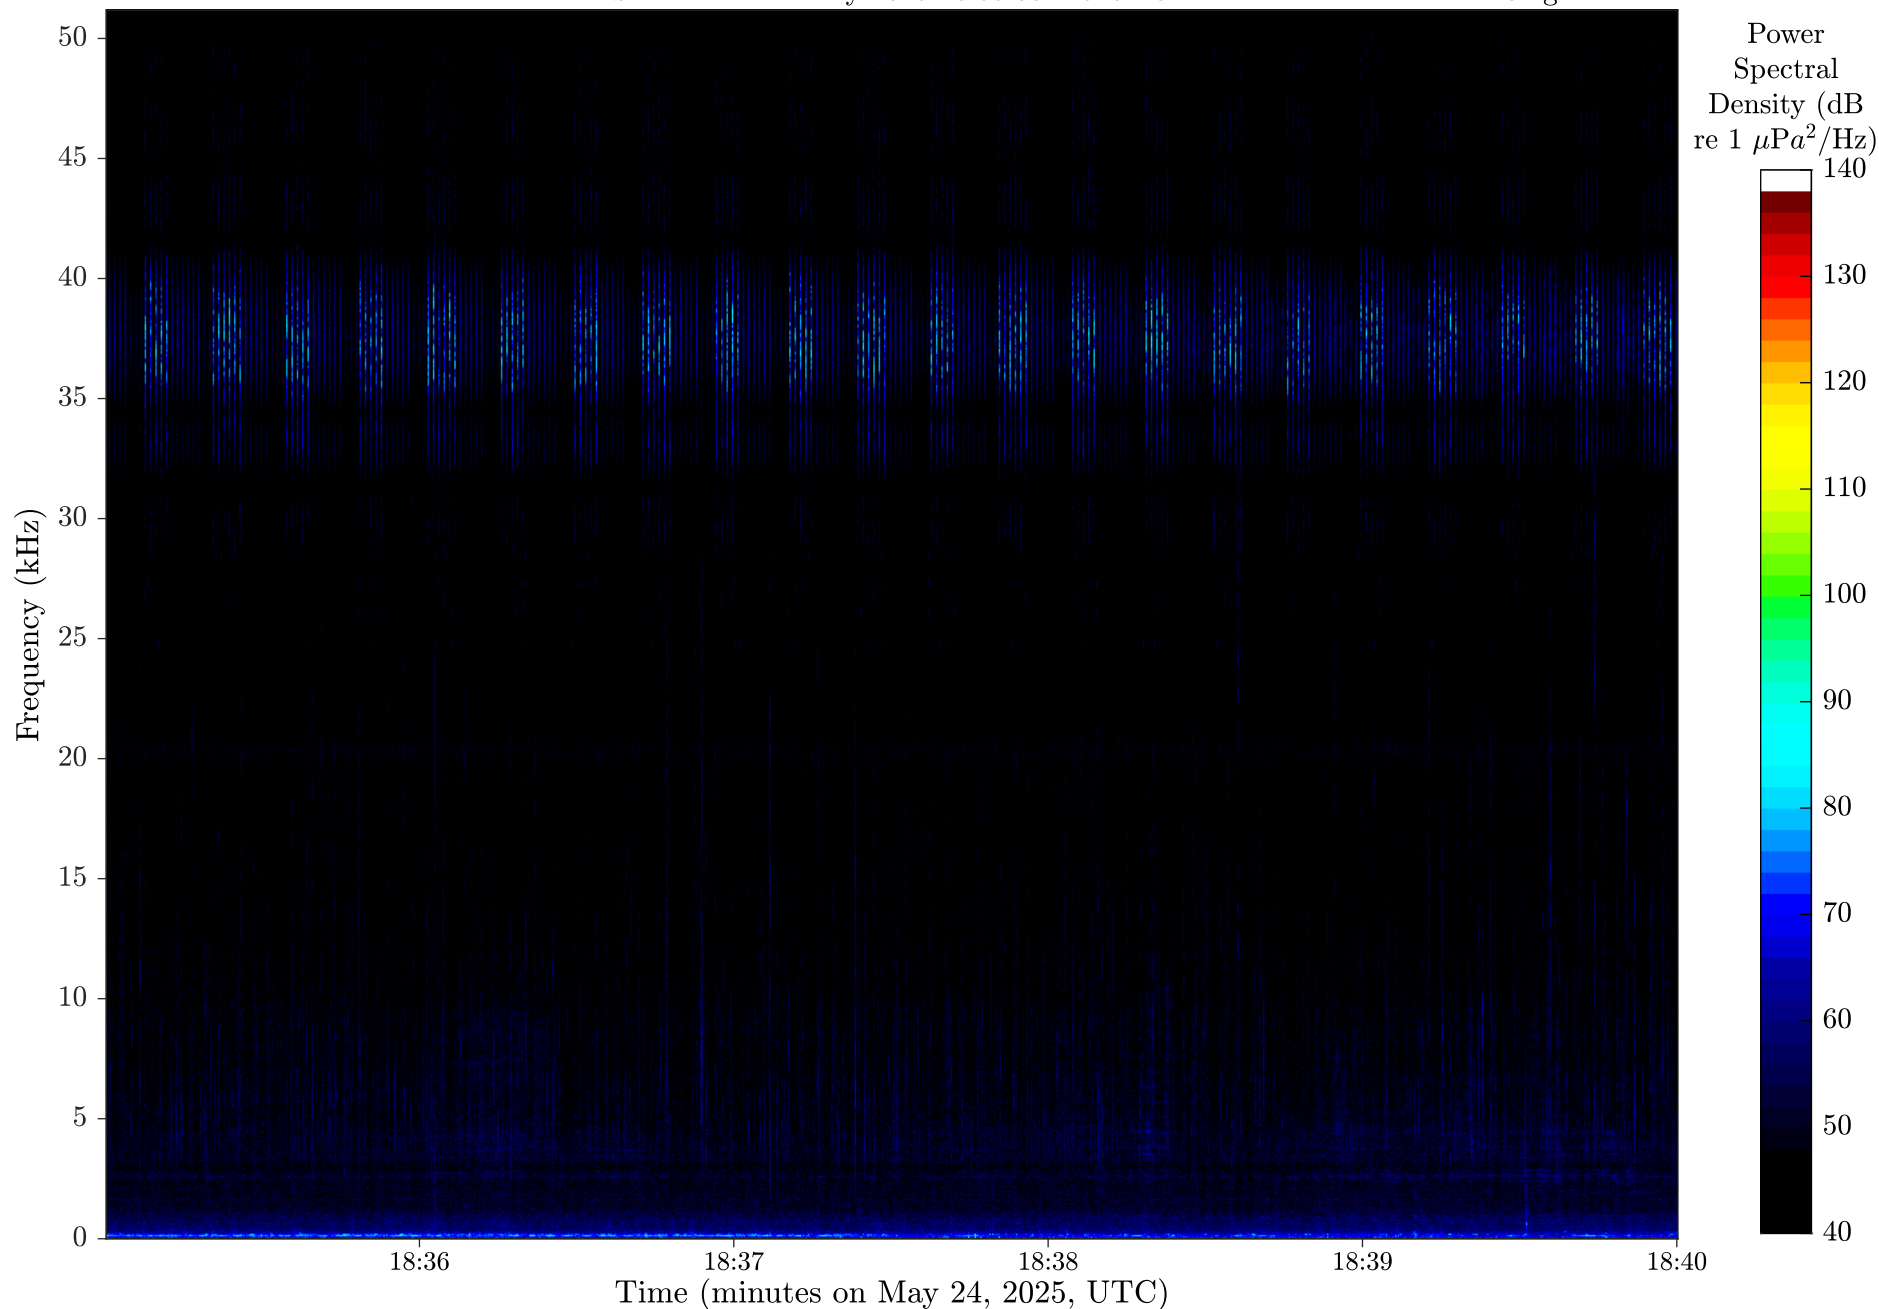


Comments: 31.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:41 UTC

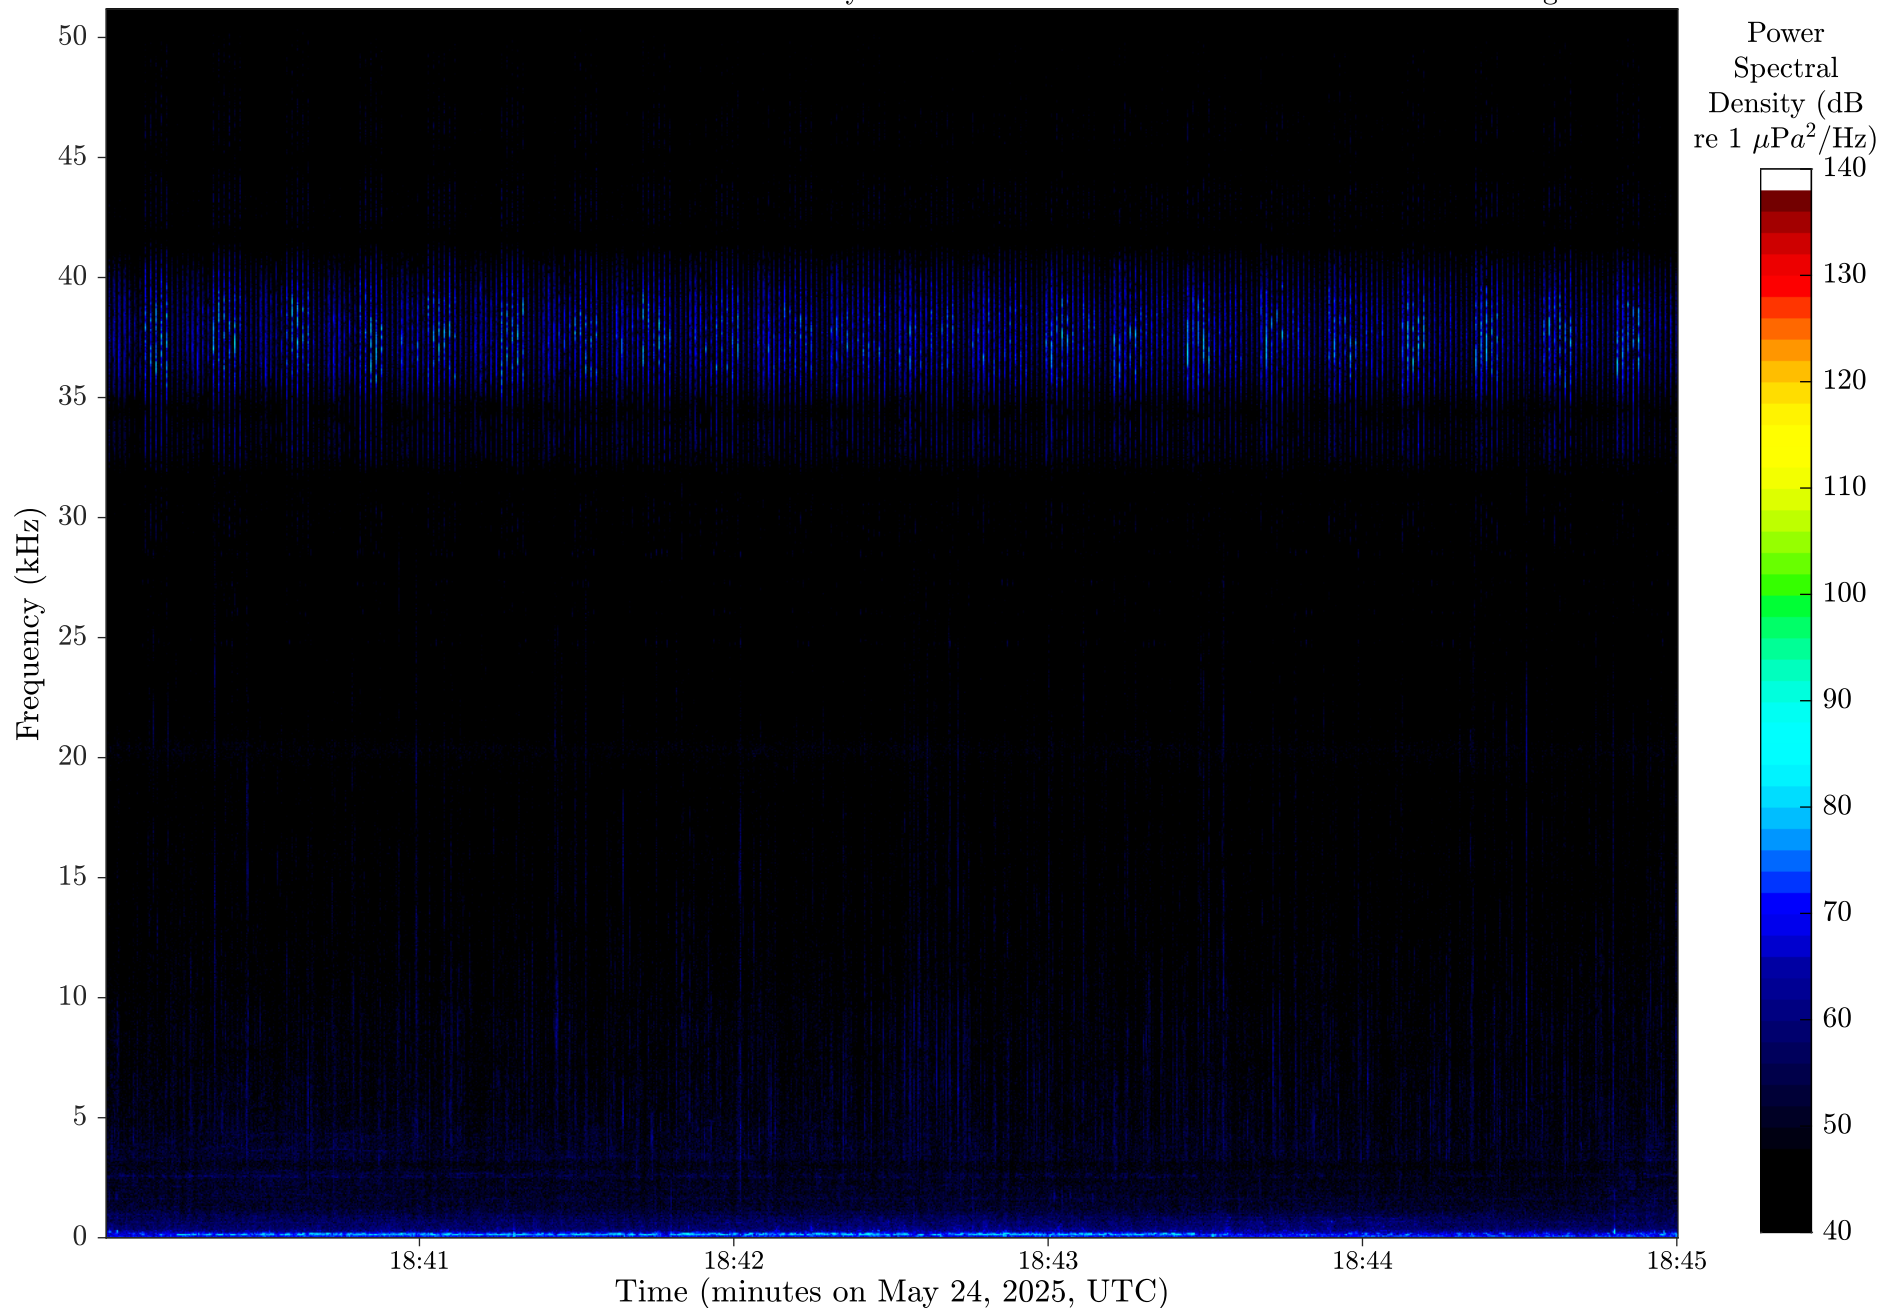


Comments: 30.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:49 UTC

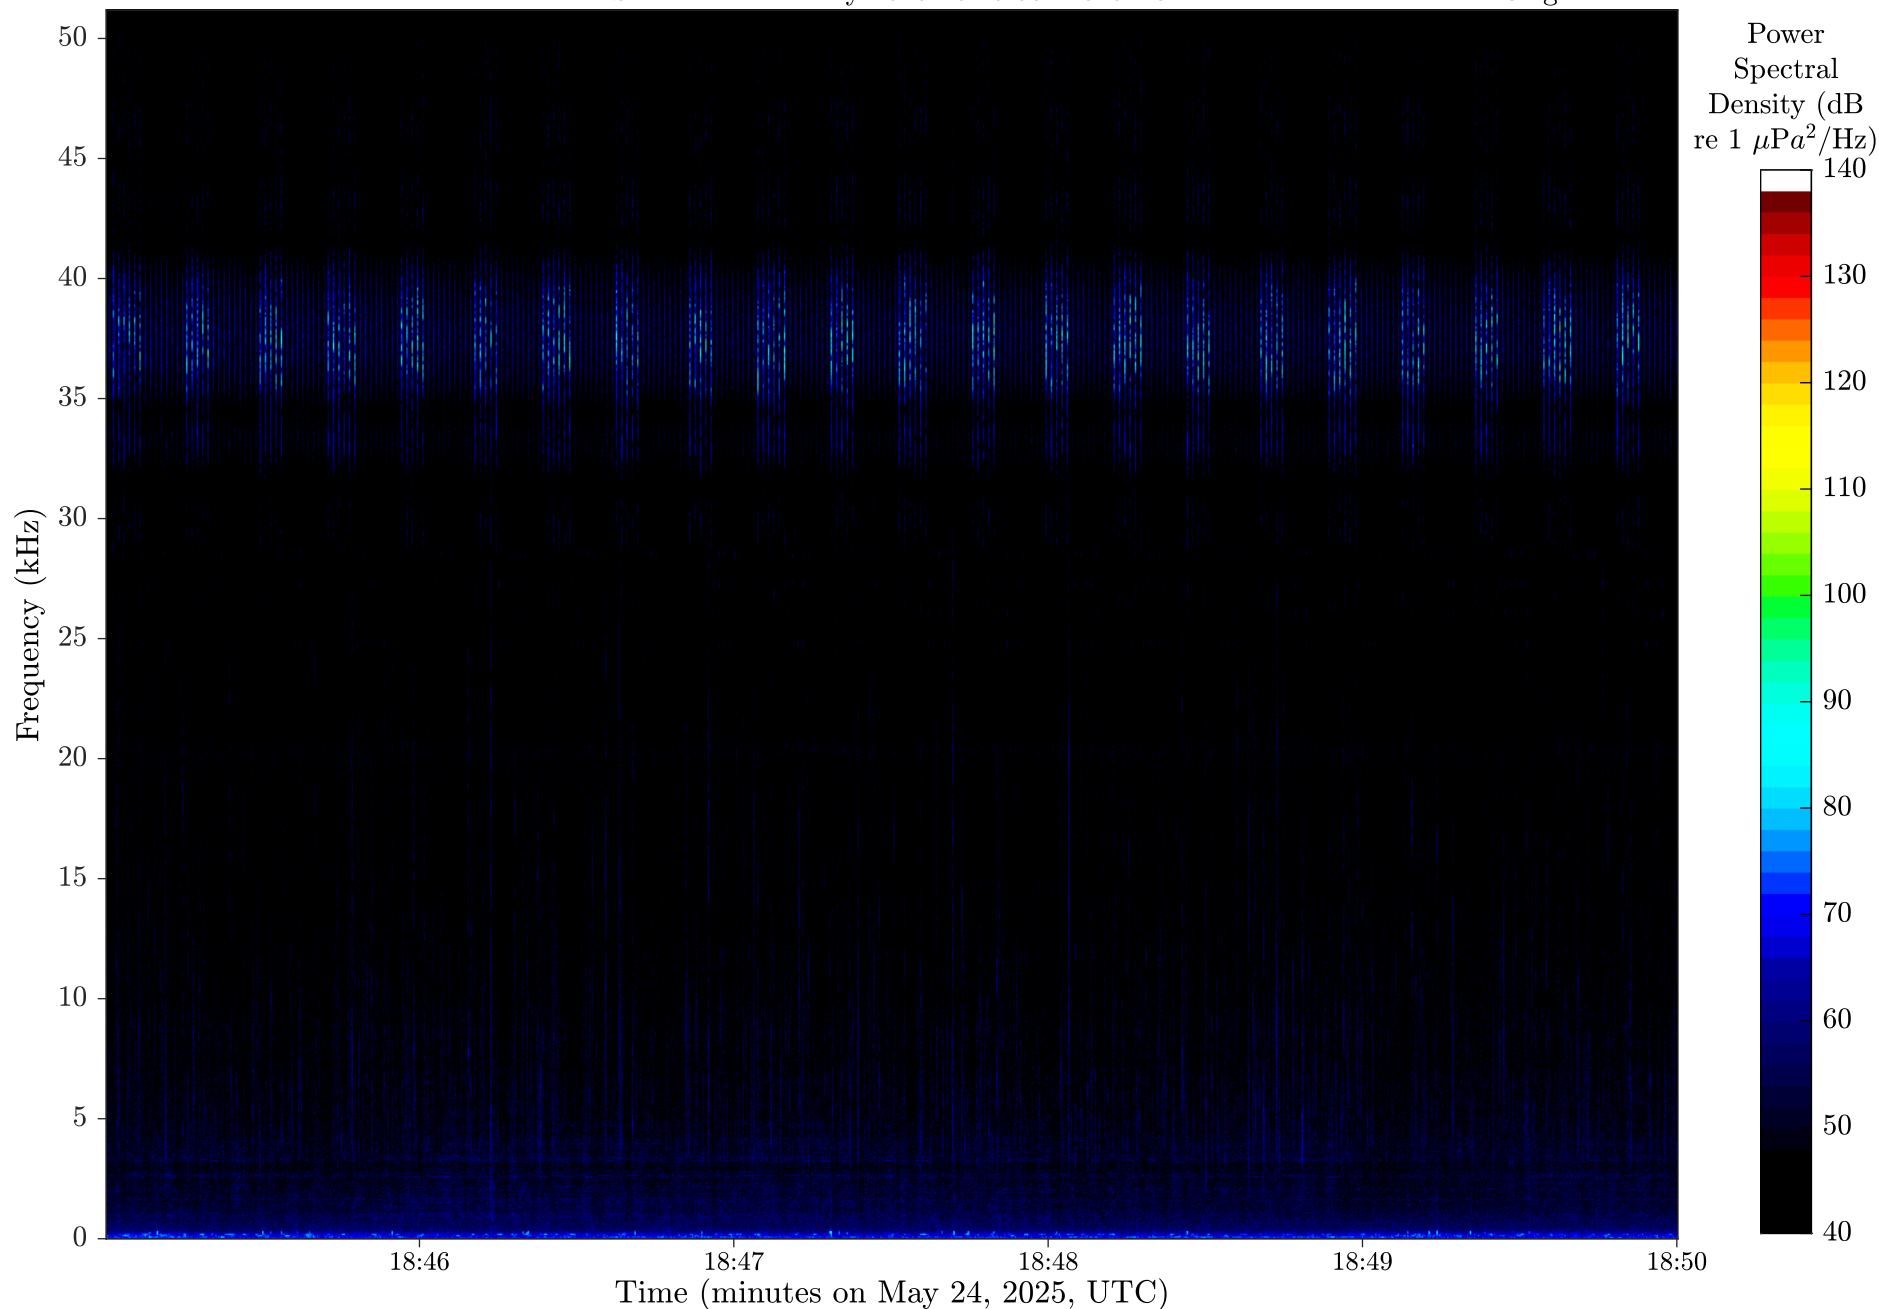


Comments: 31.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:57 UTC

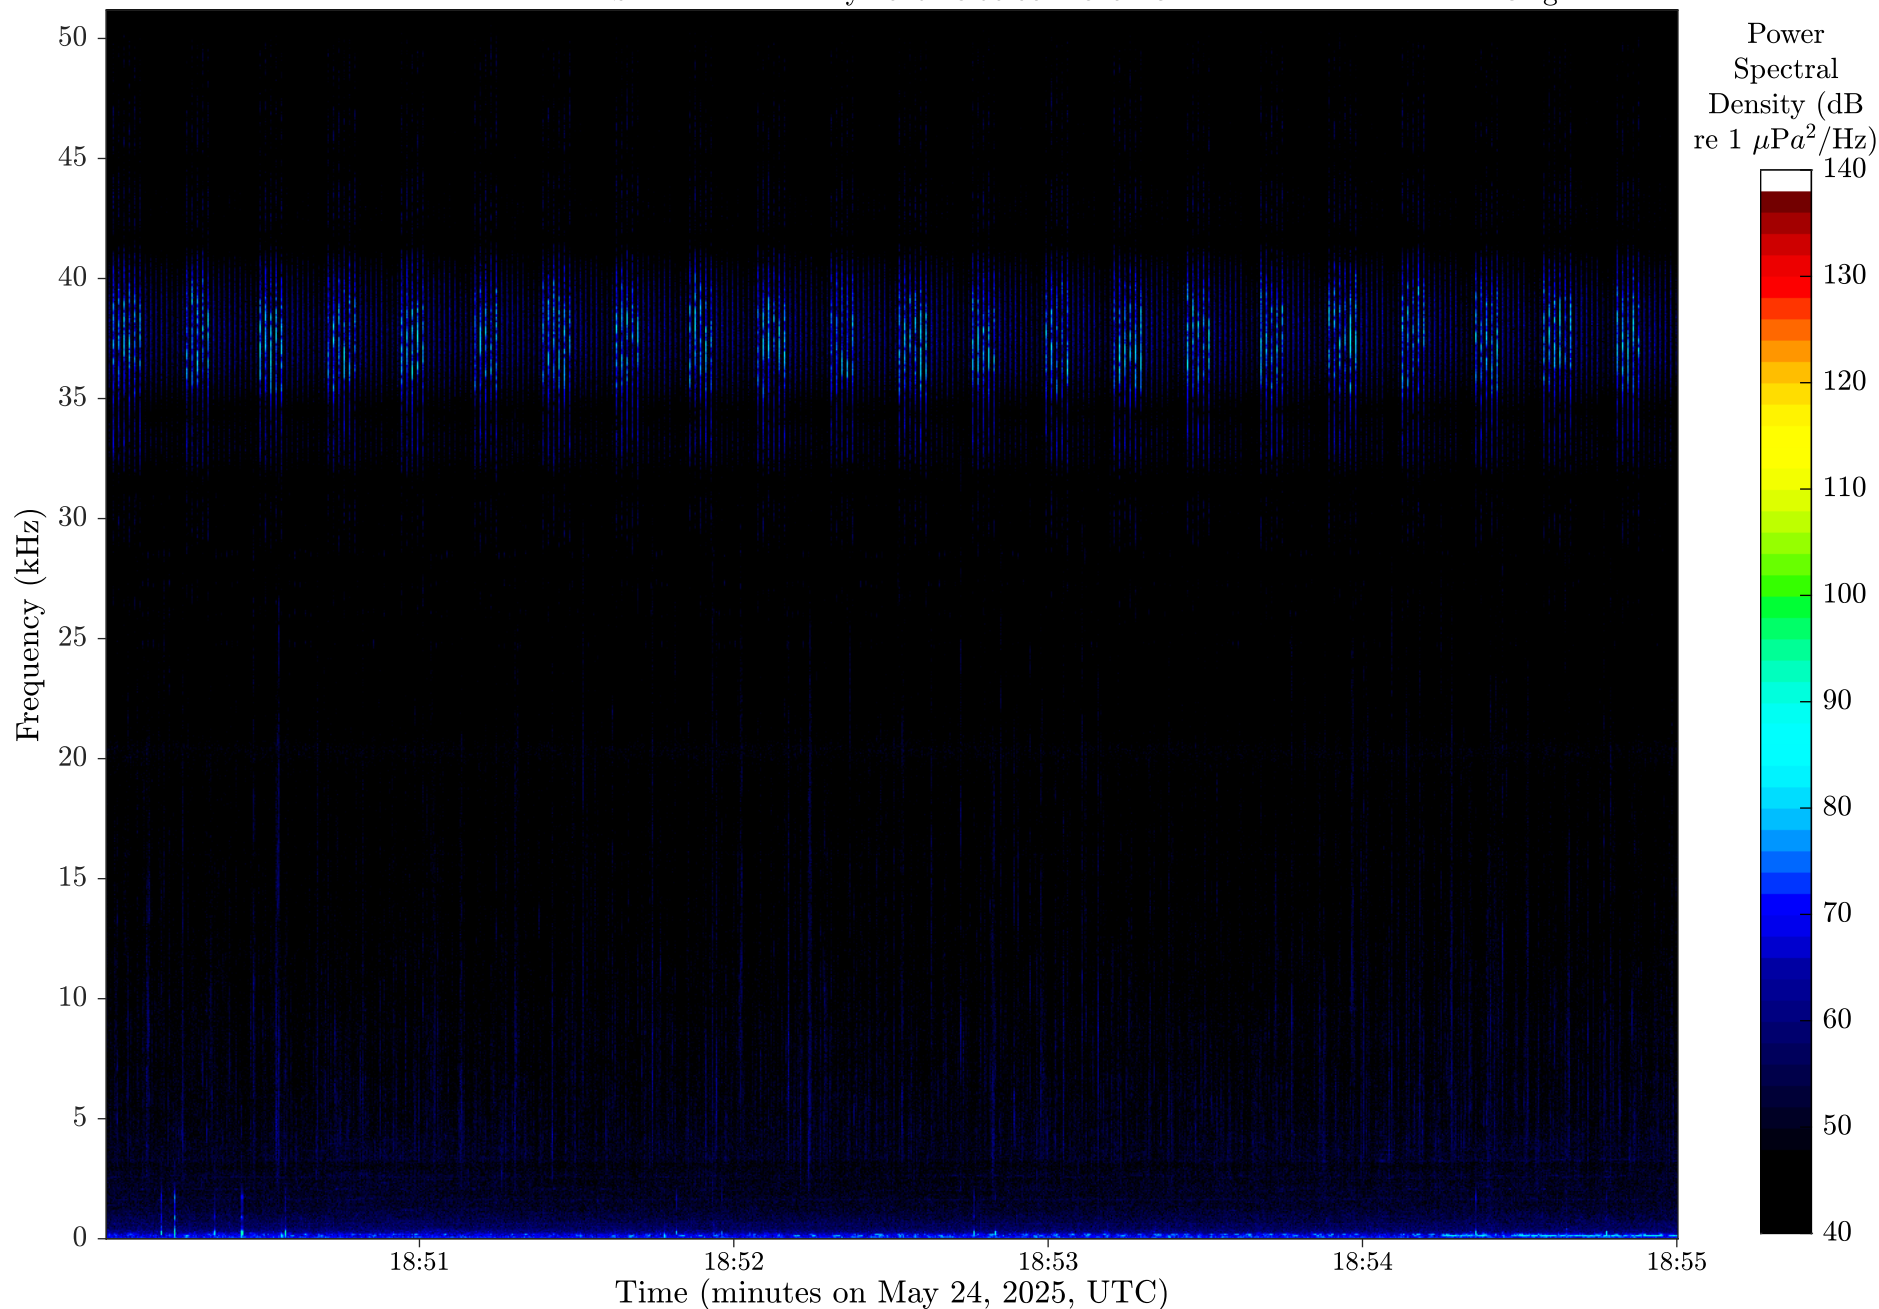


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:05 UTC

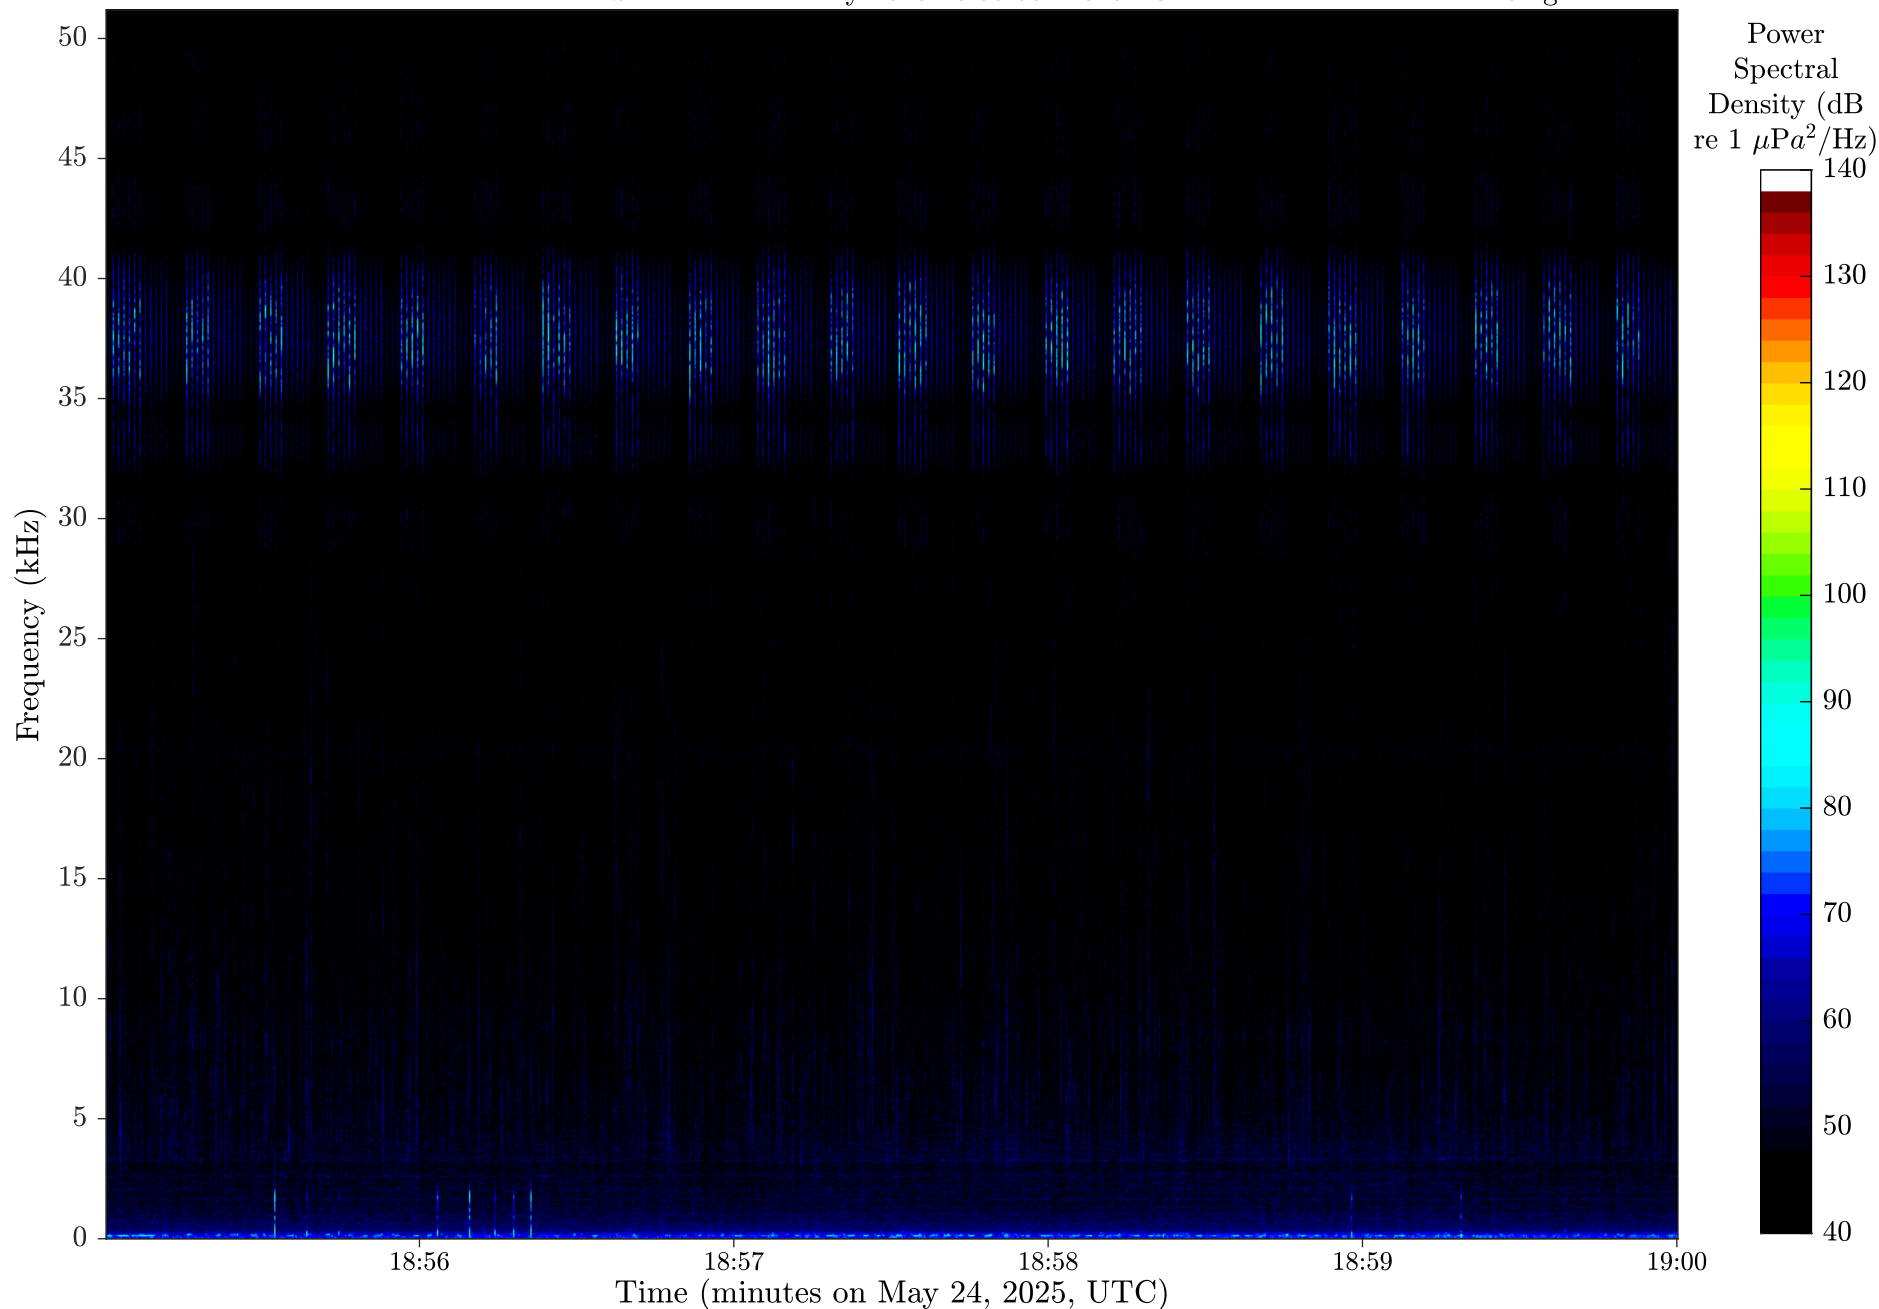


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:12 UTC

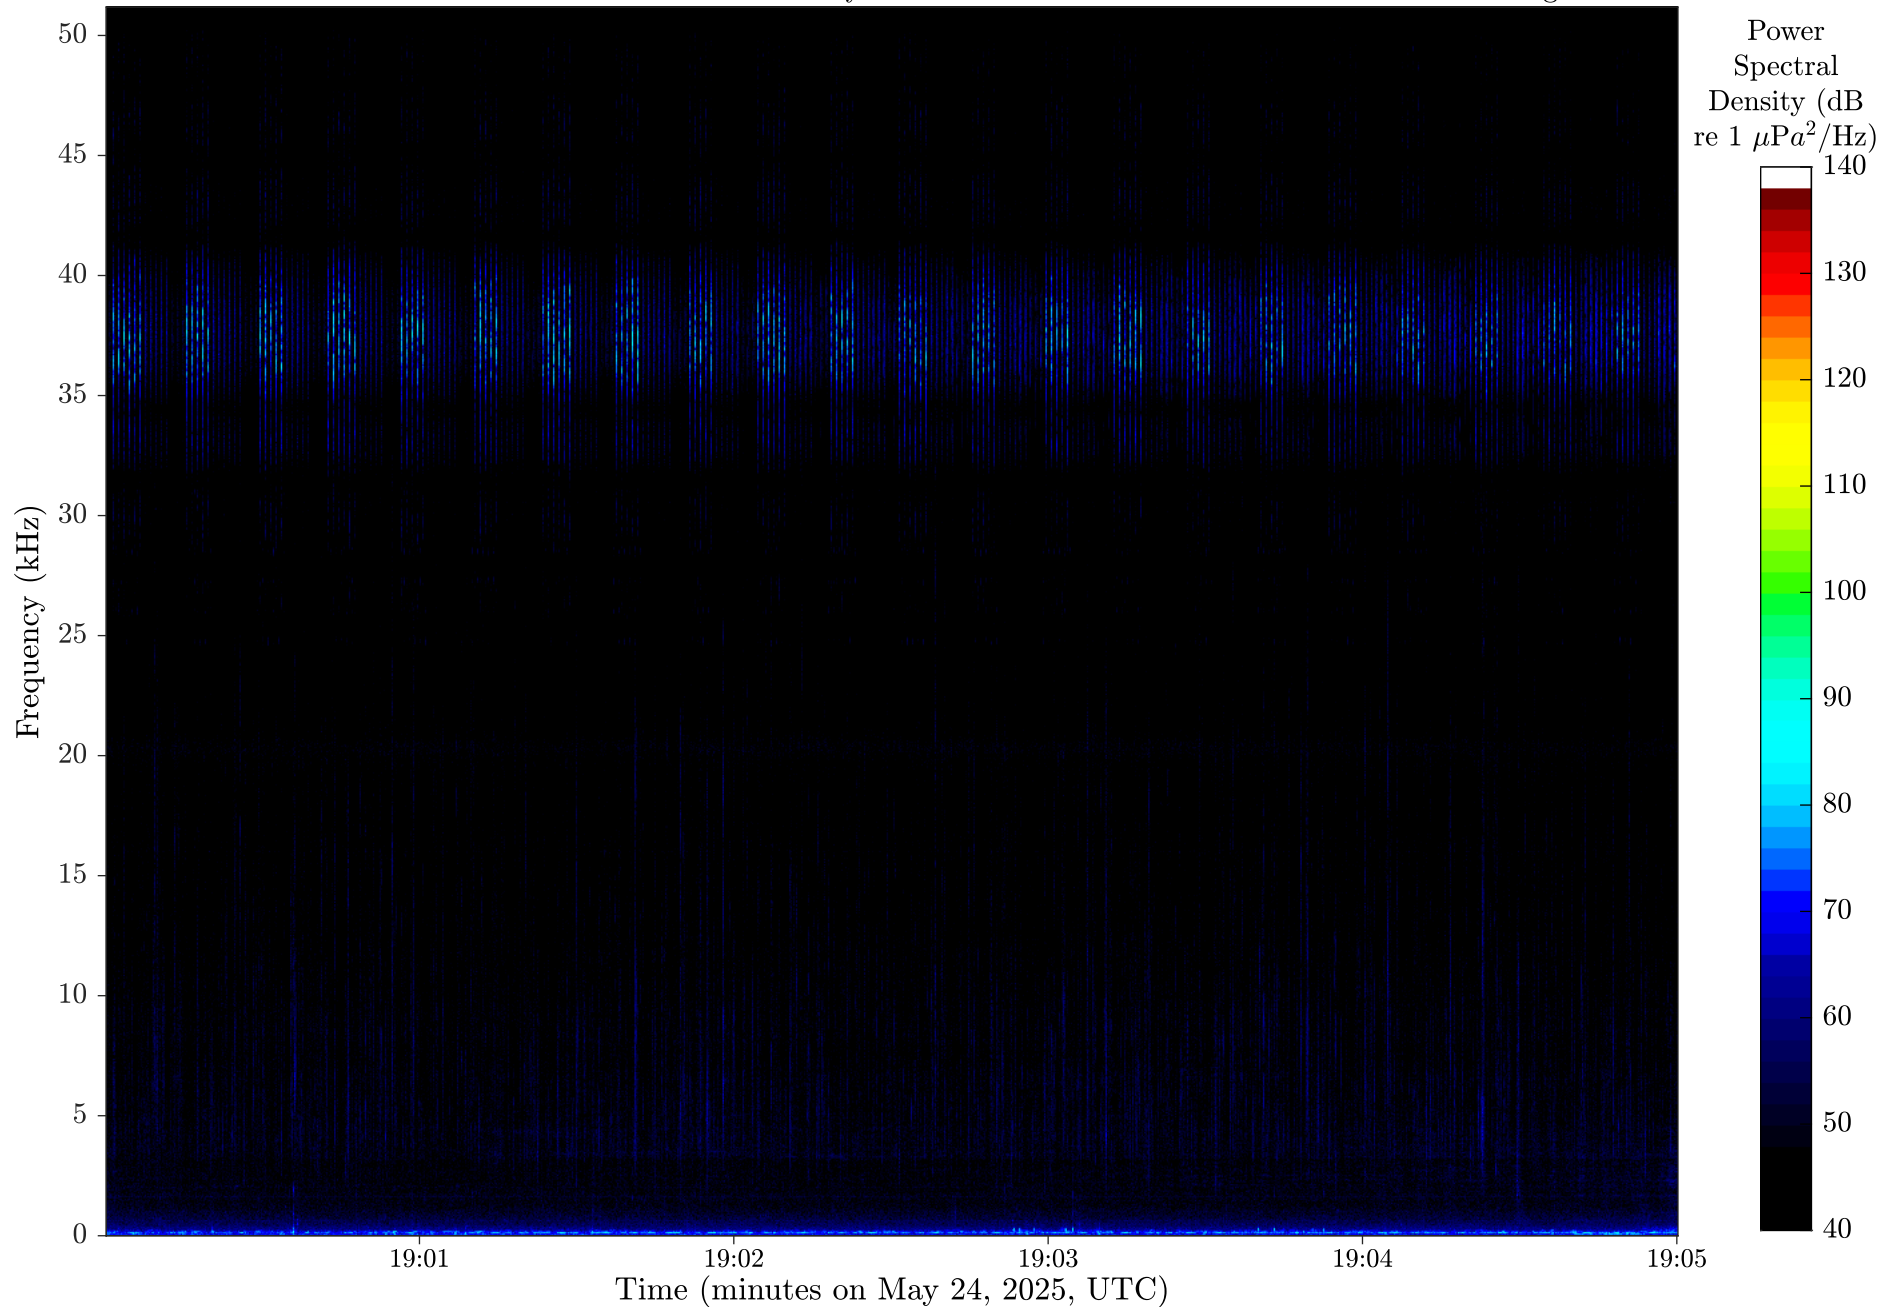


Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:38:20 UTC

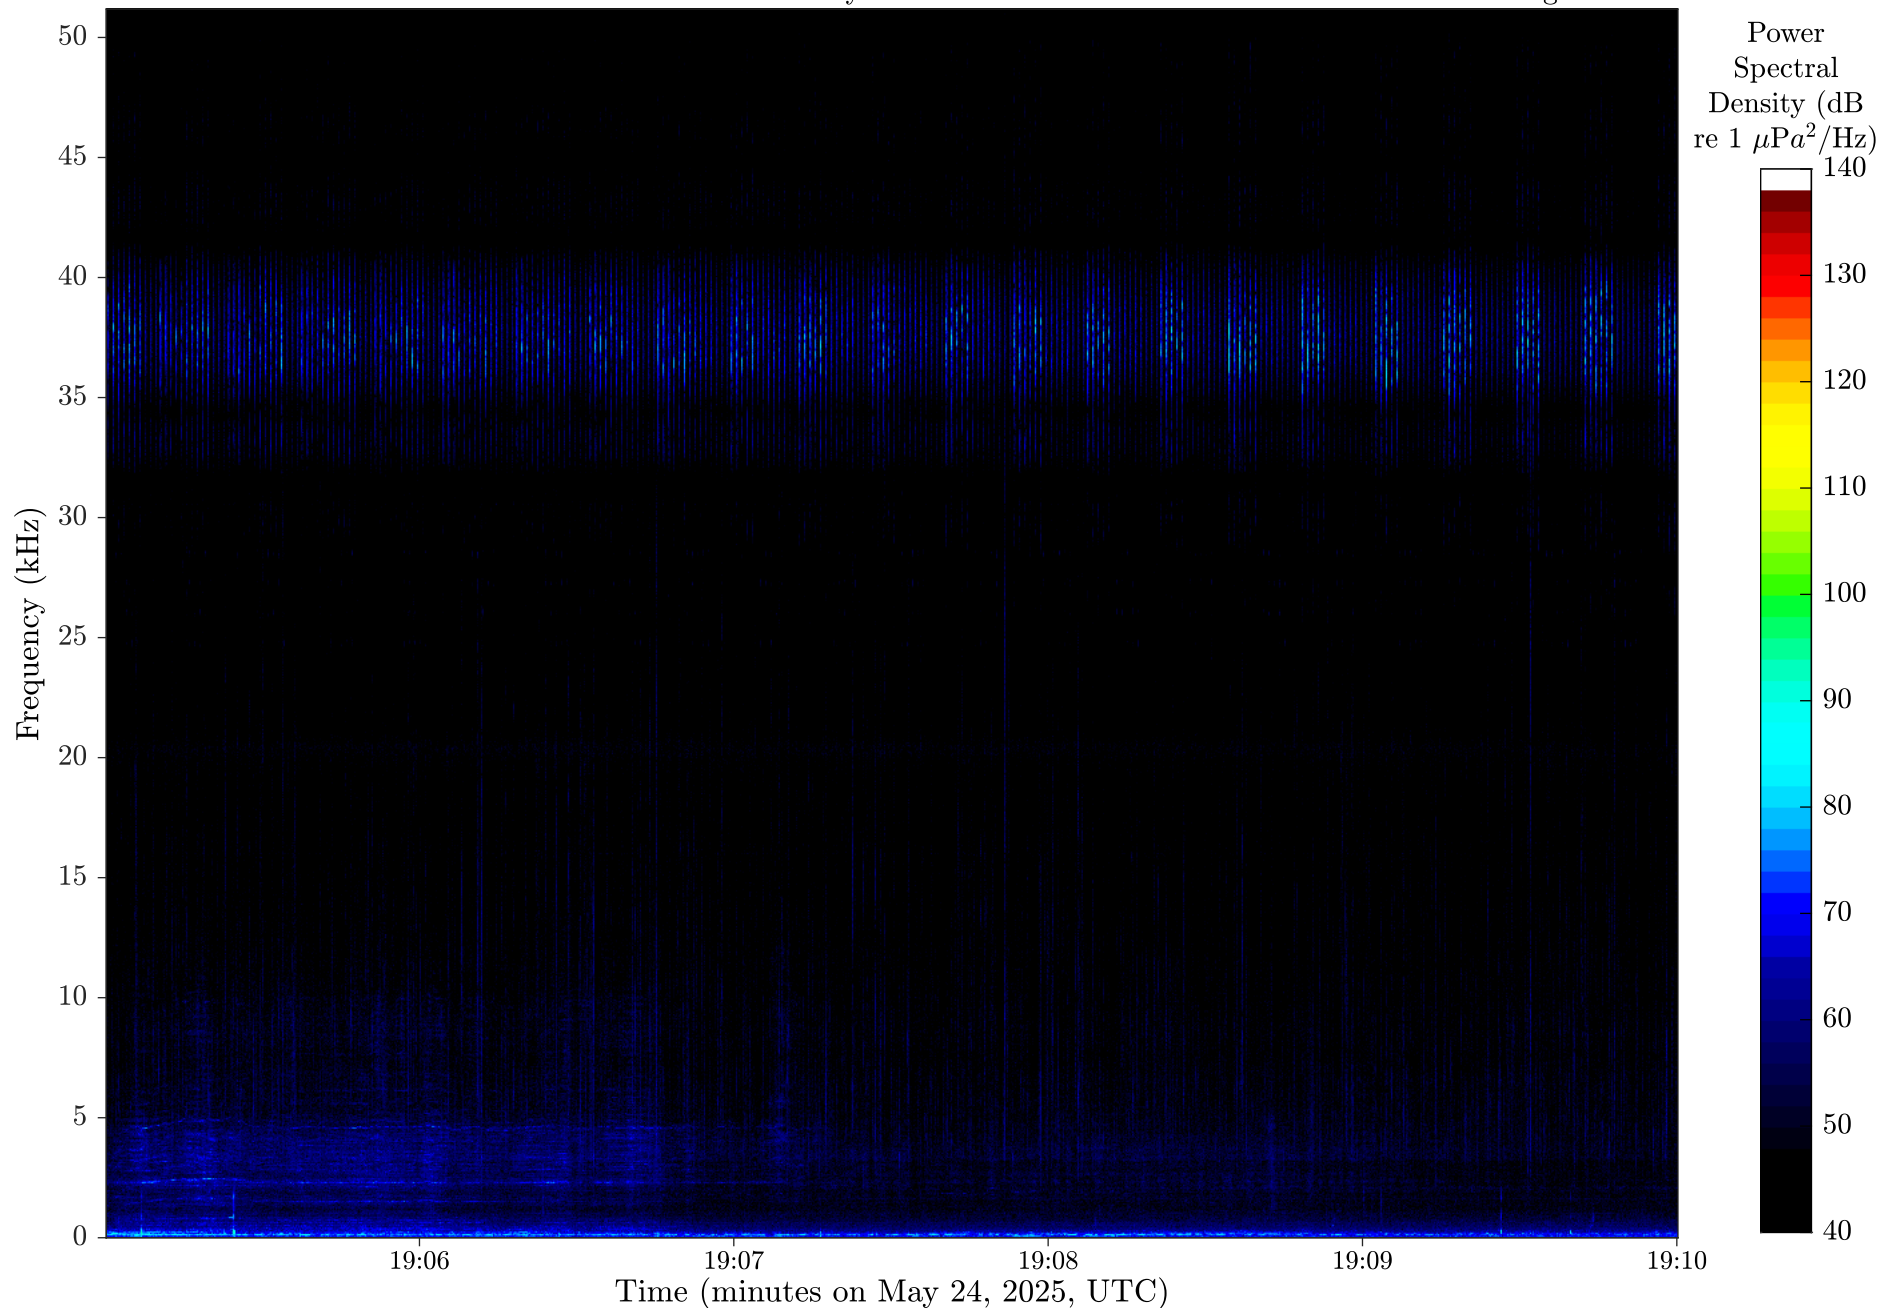


Comments: 32.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:29 UTC

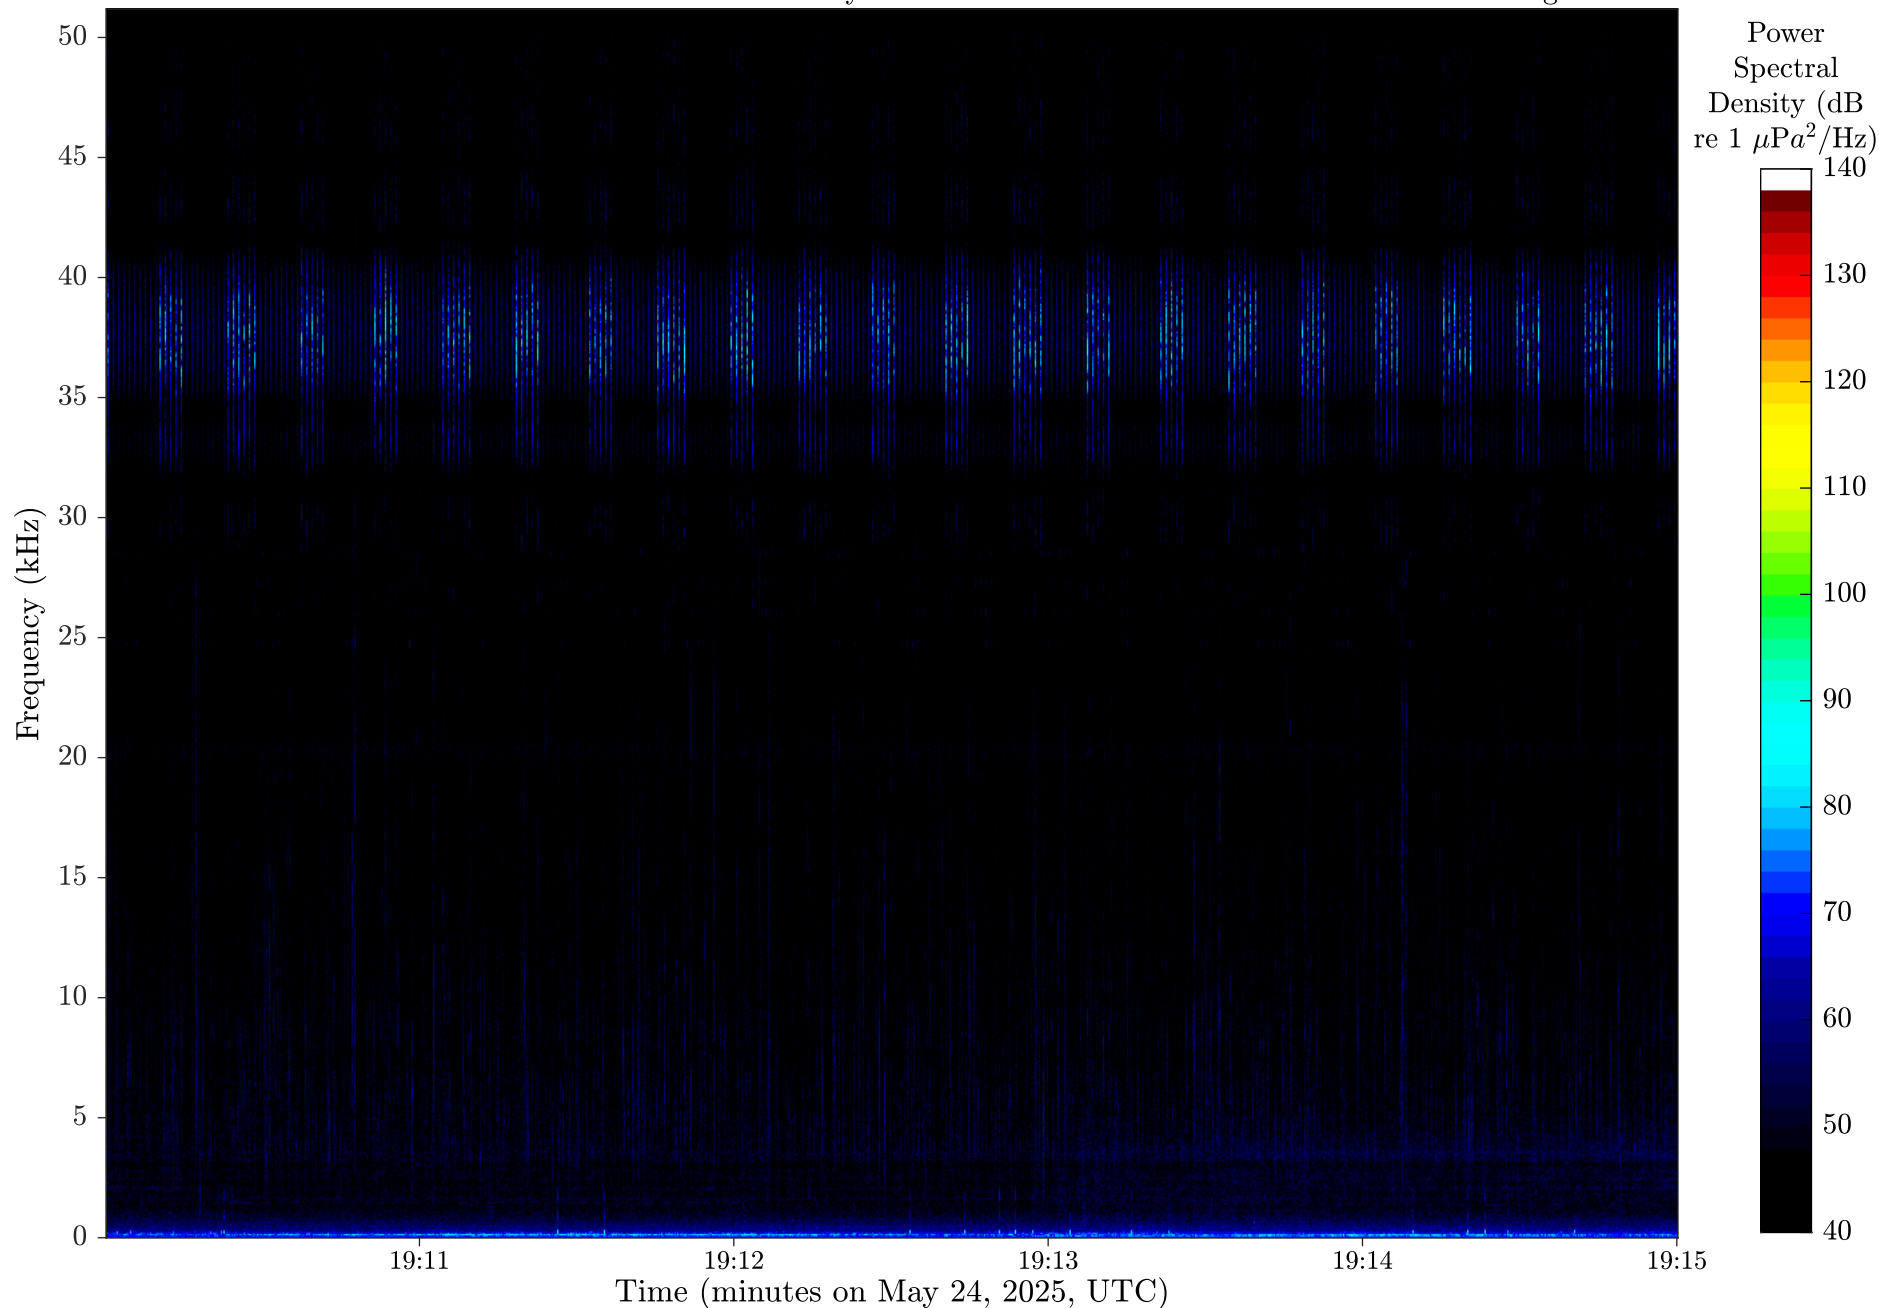


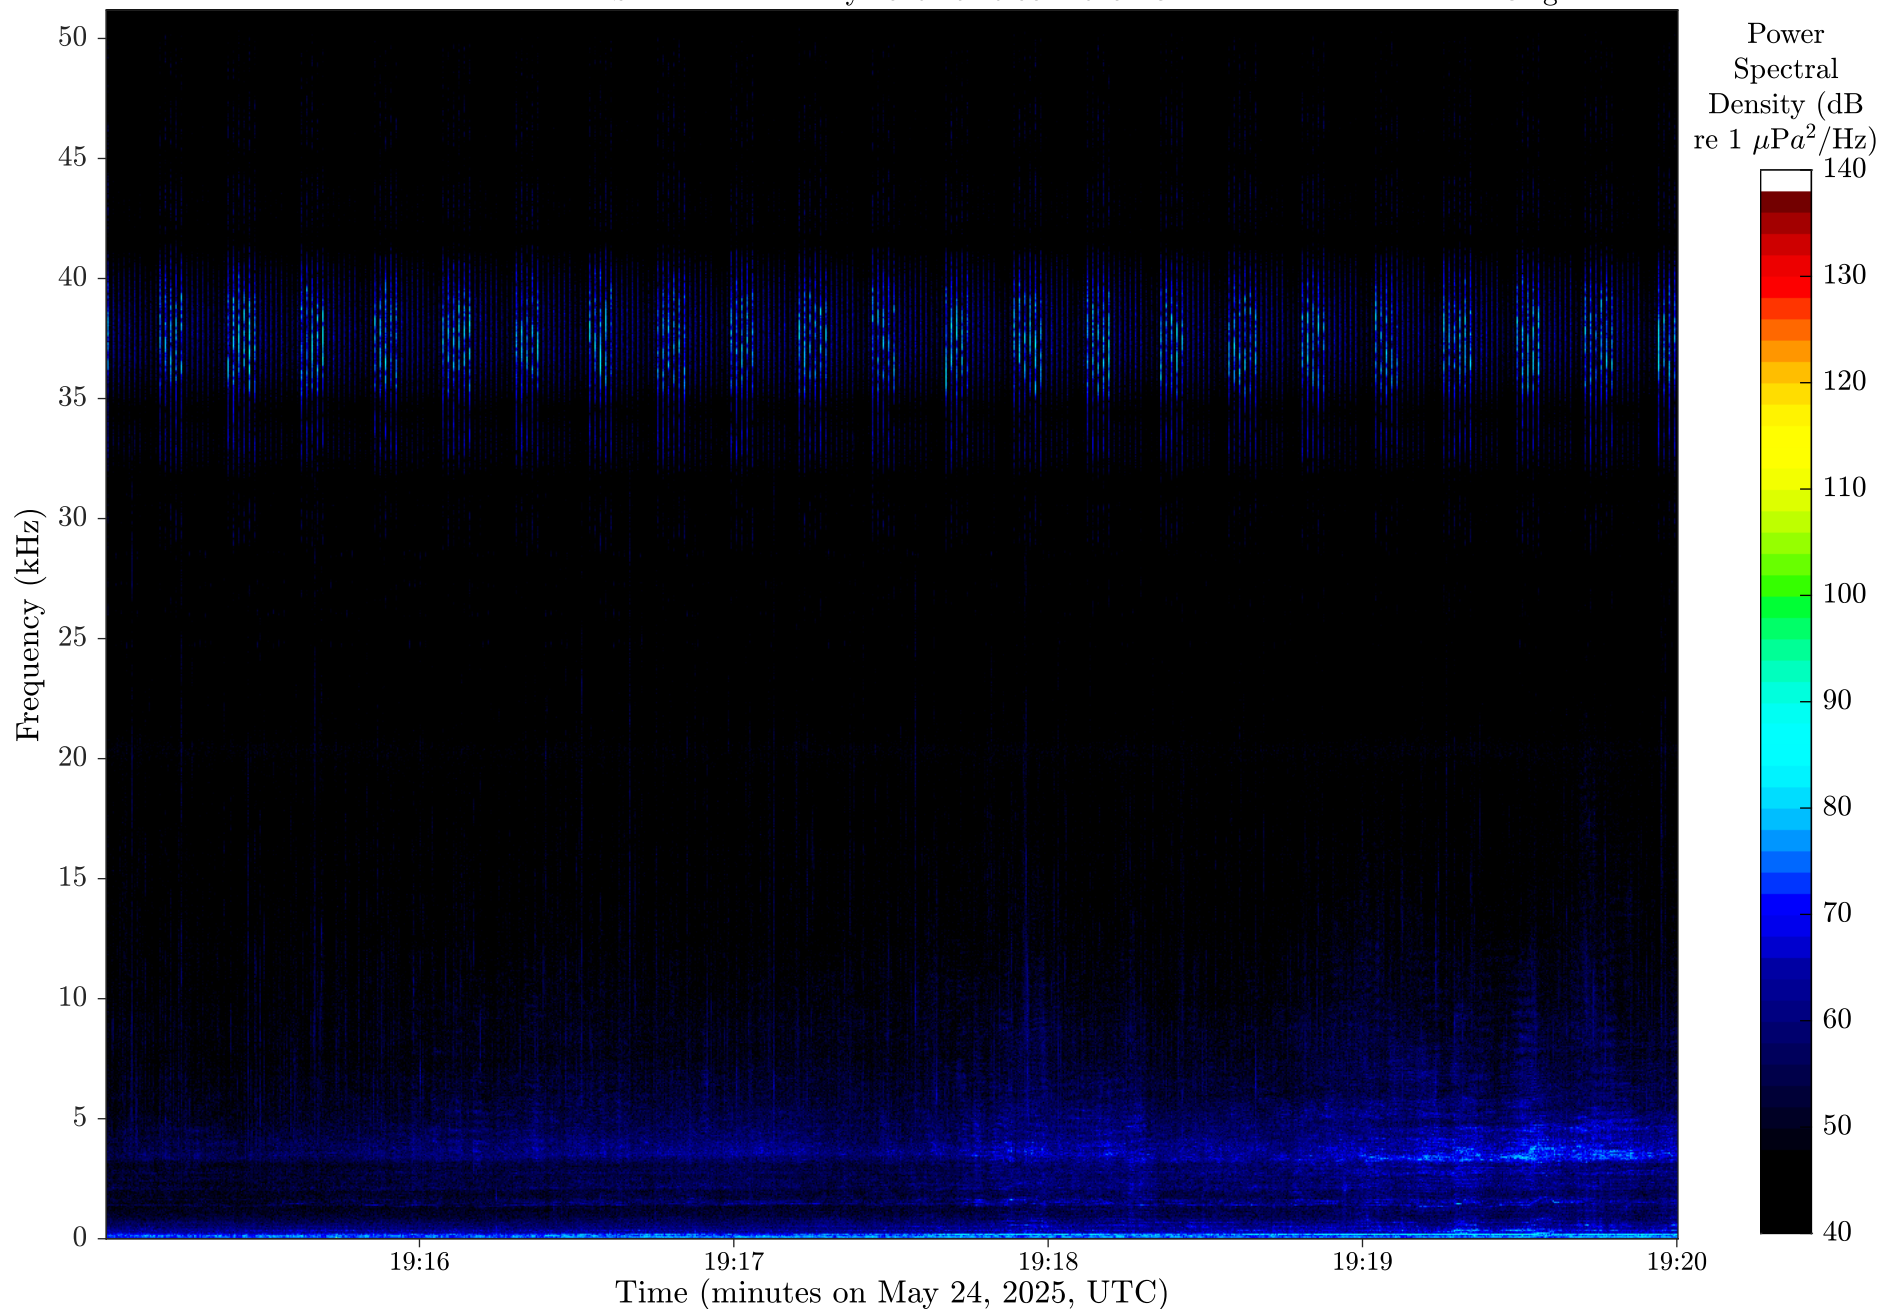

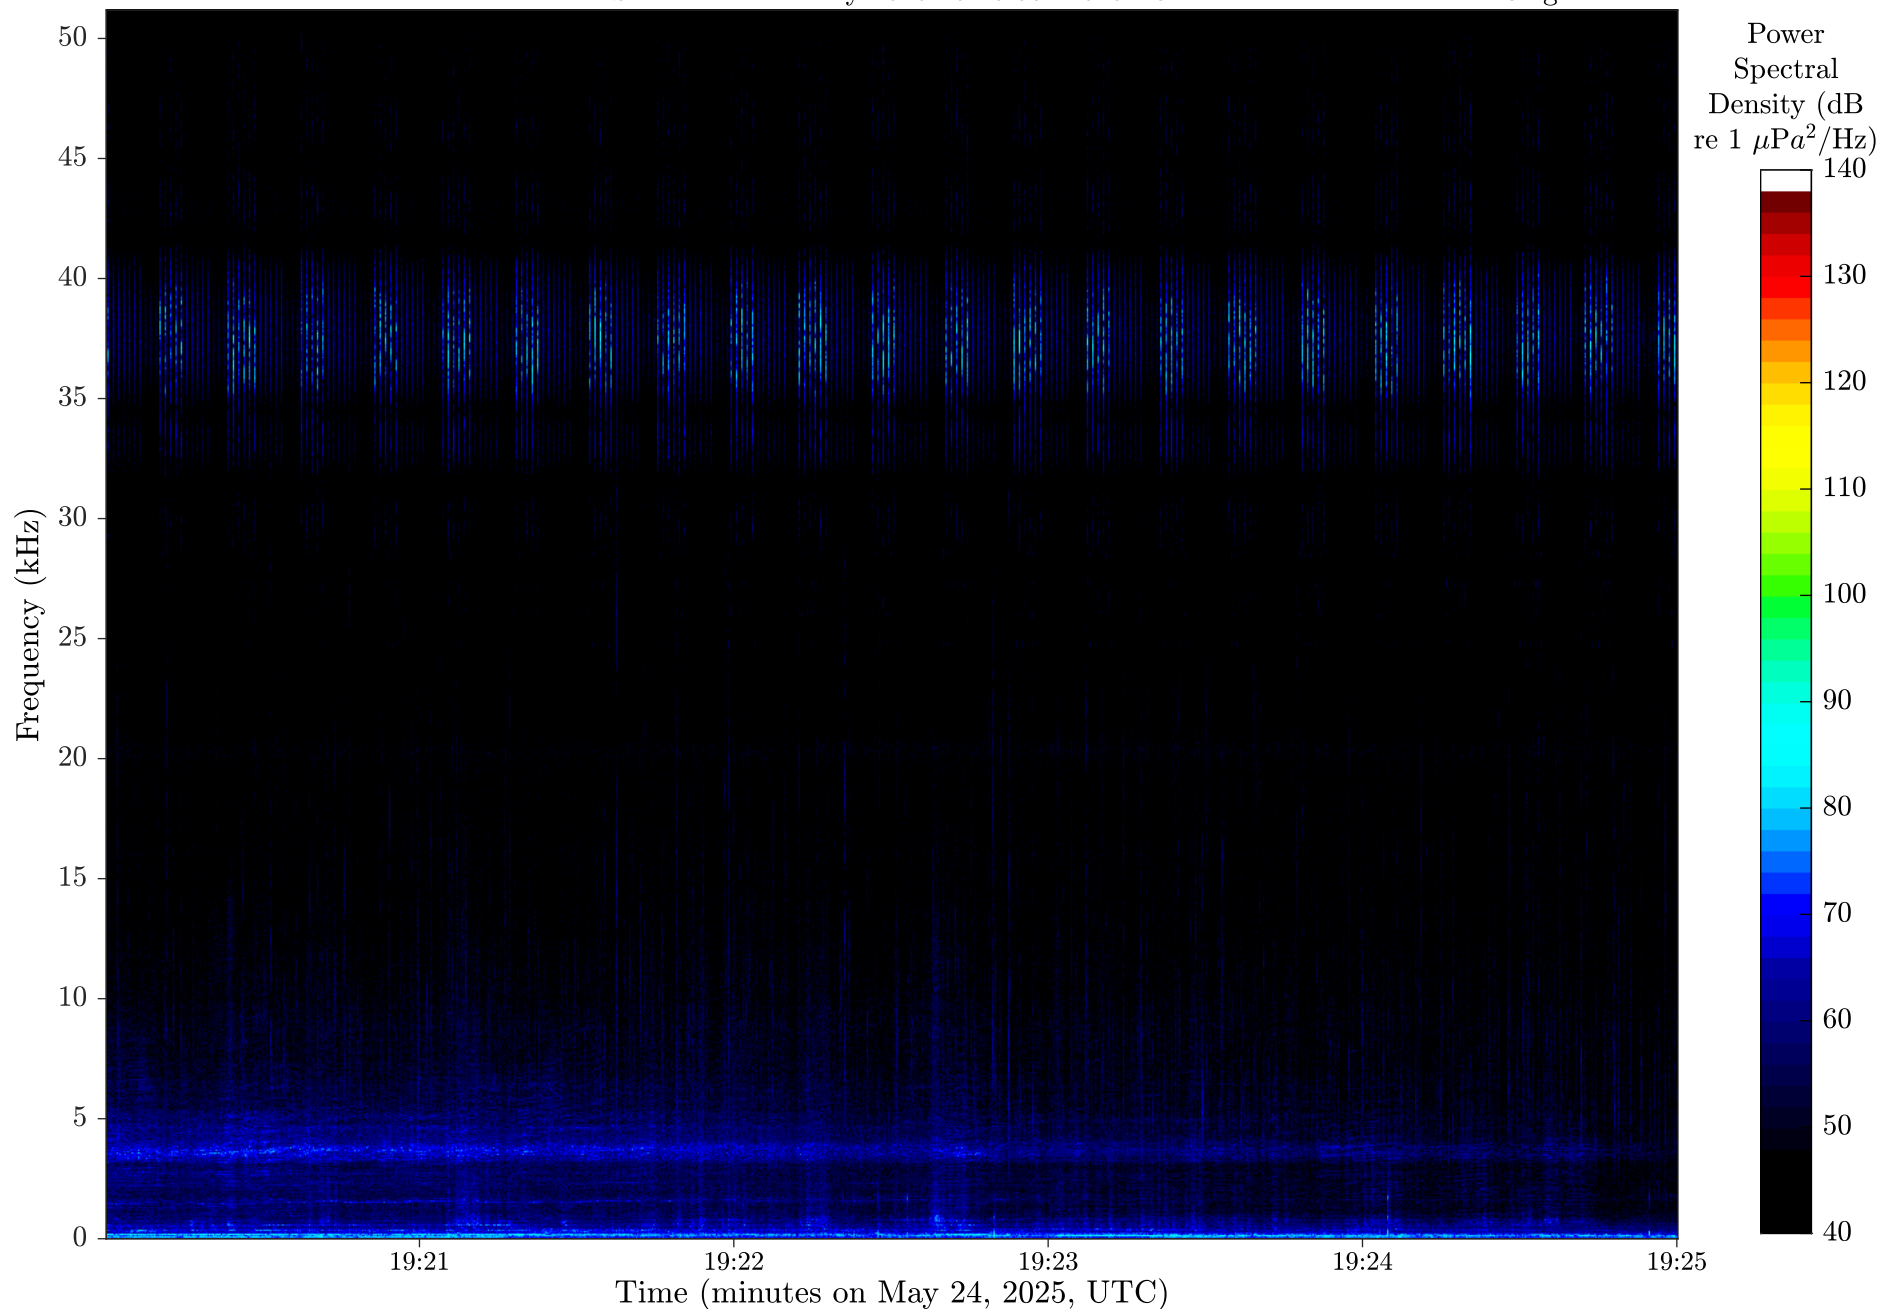


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:55 UTC

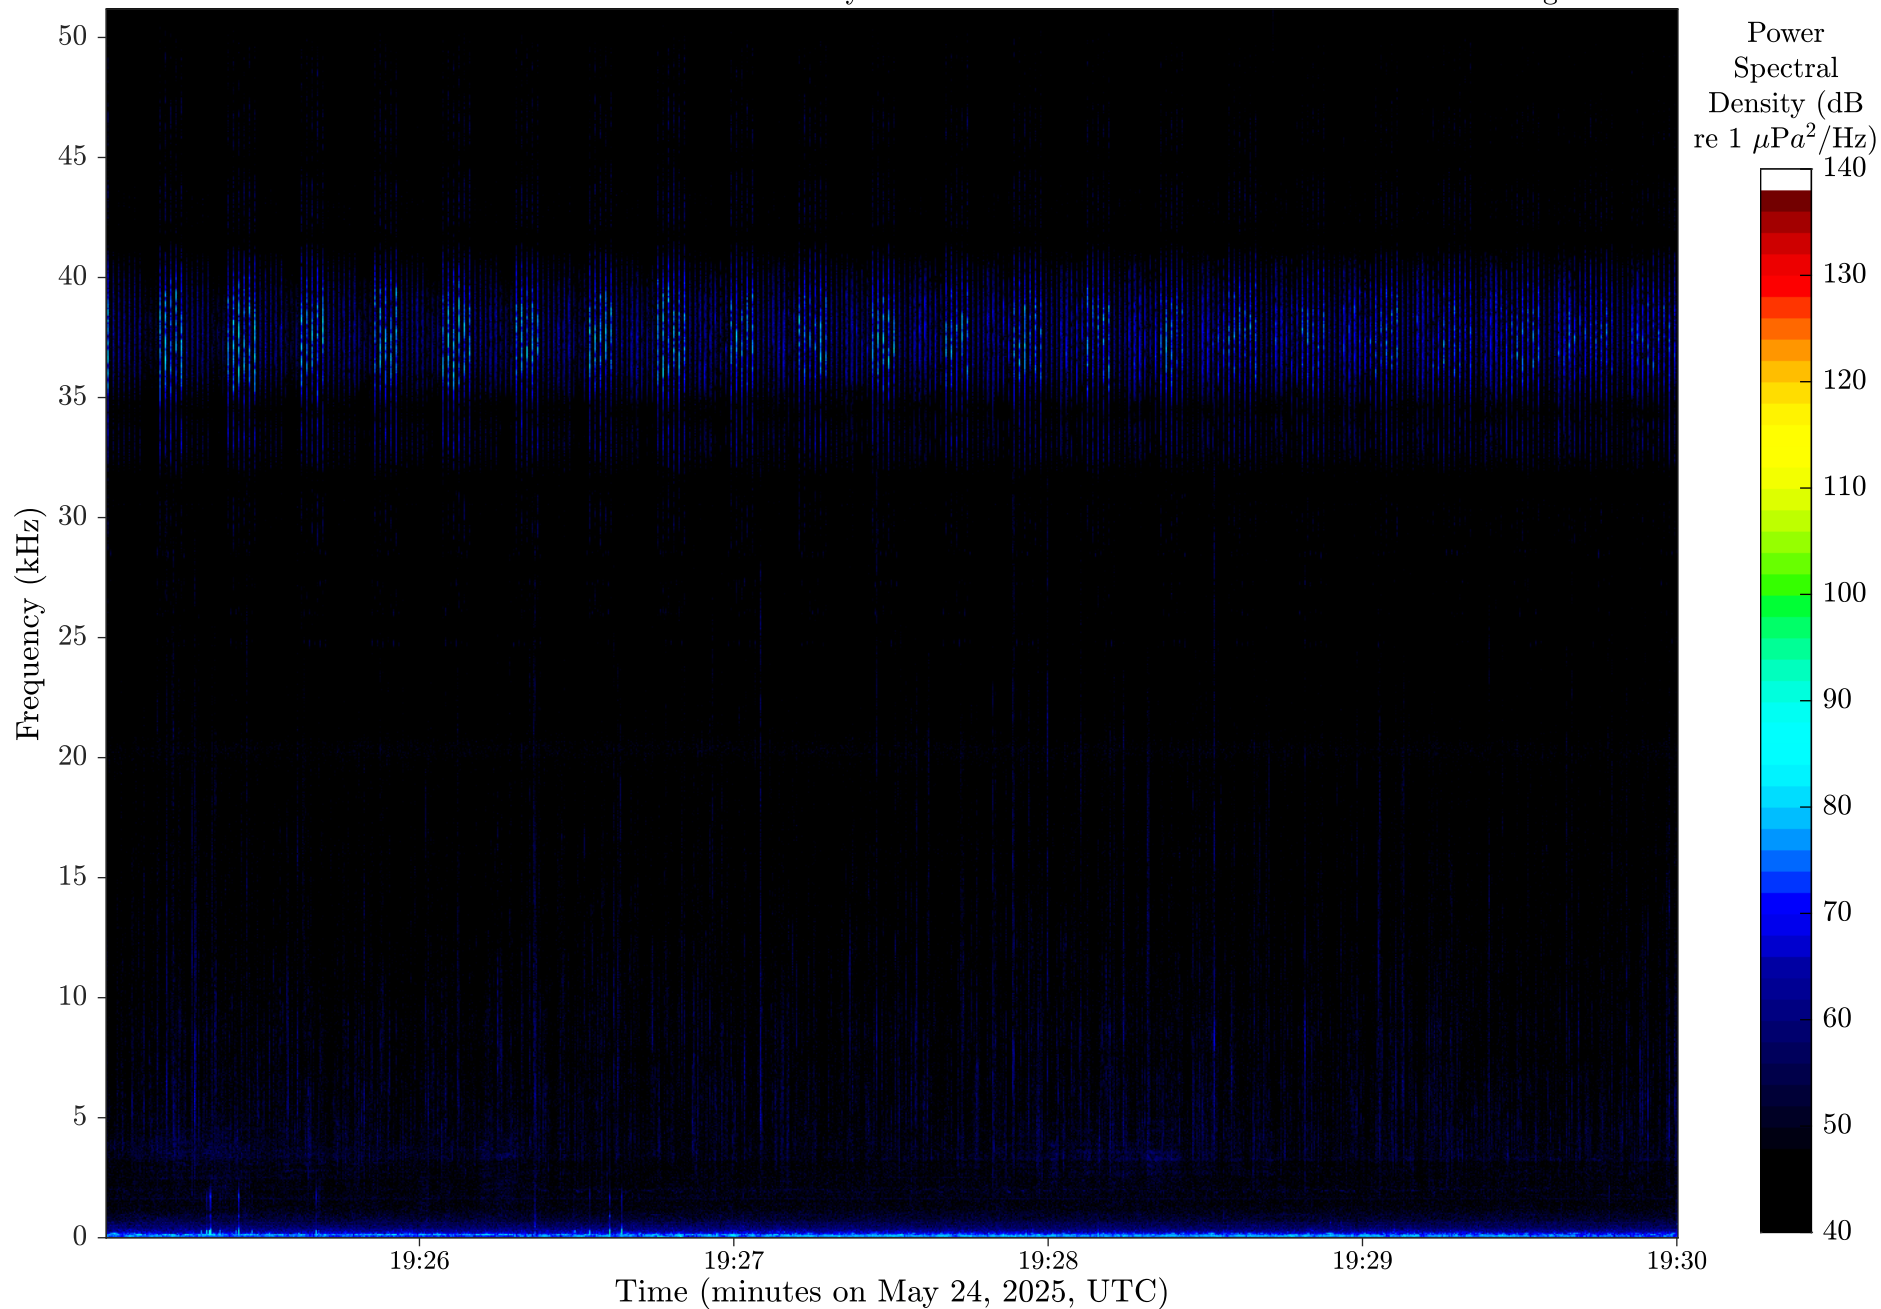


Comments: 33.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:04 UTC

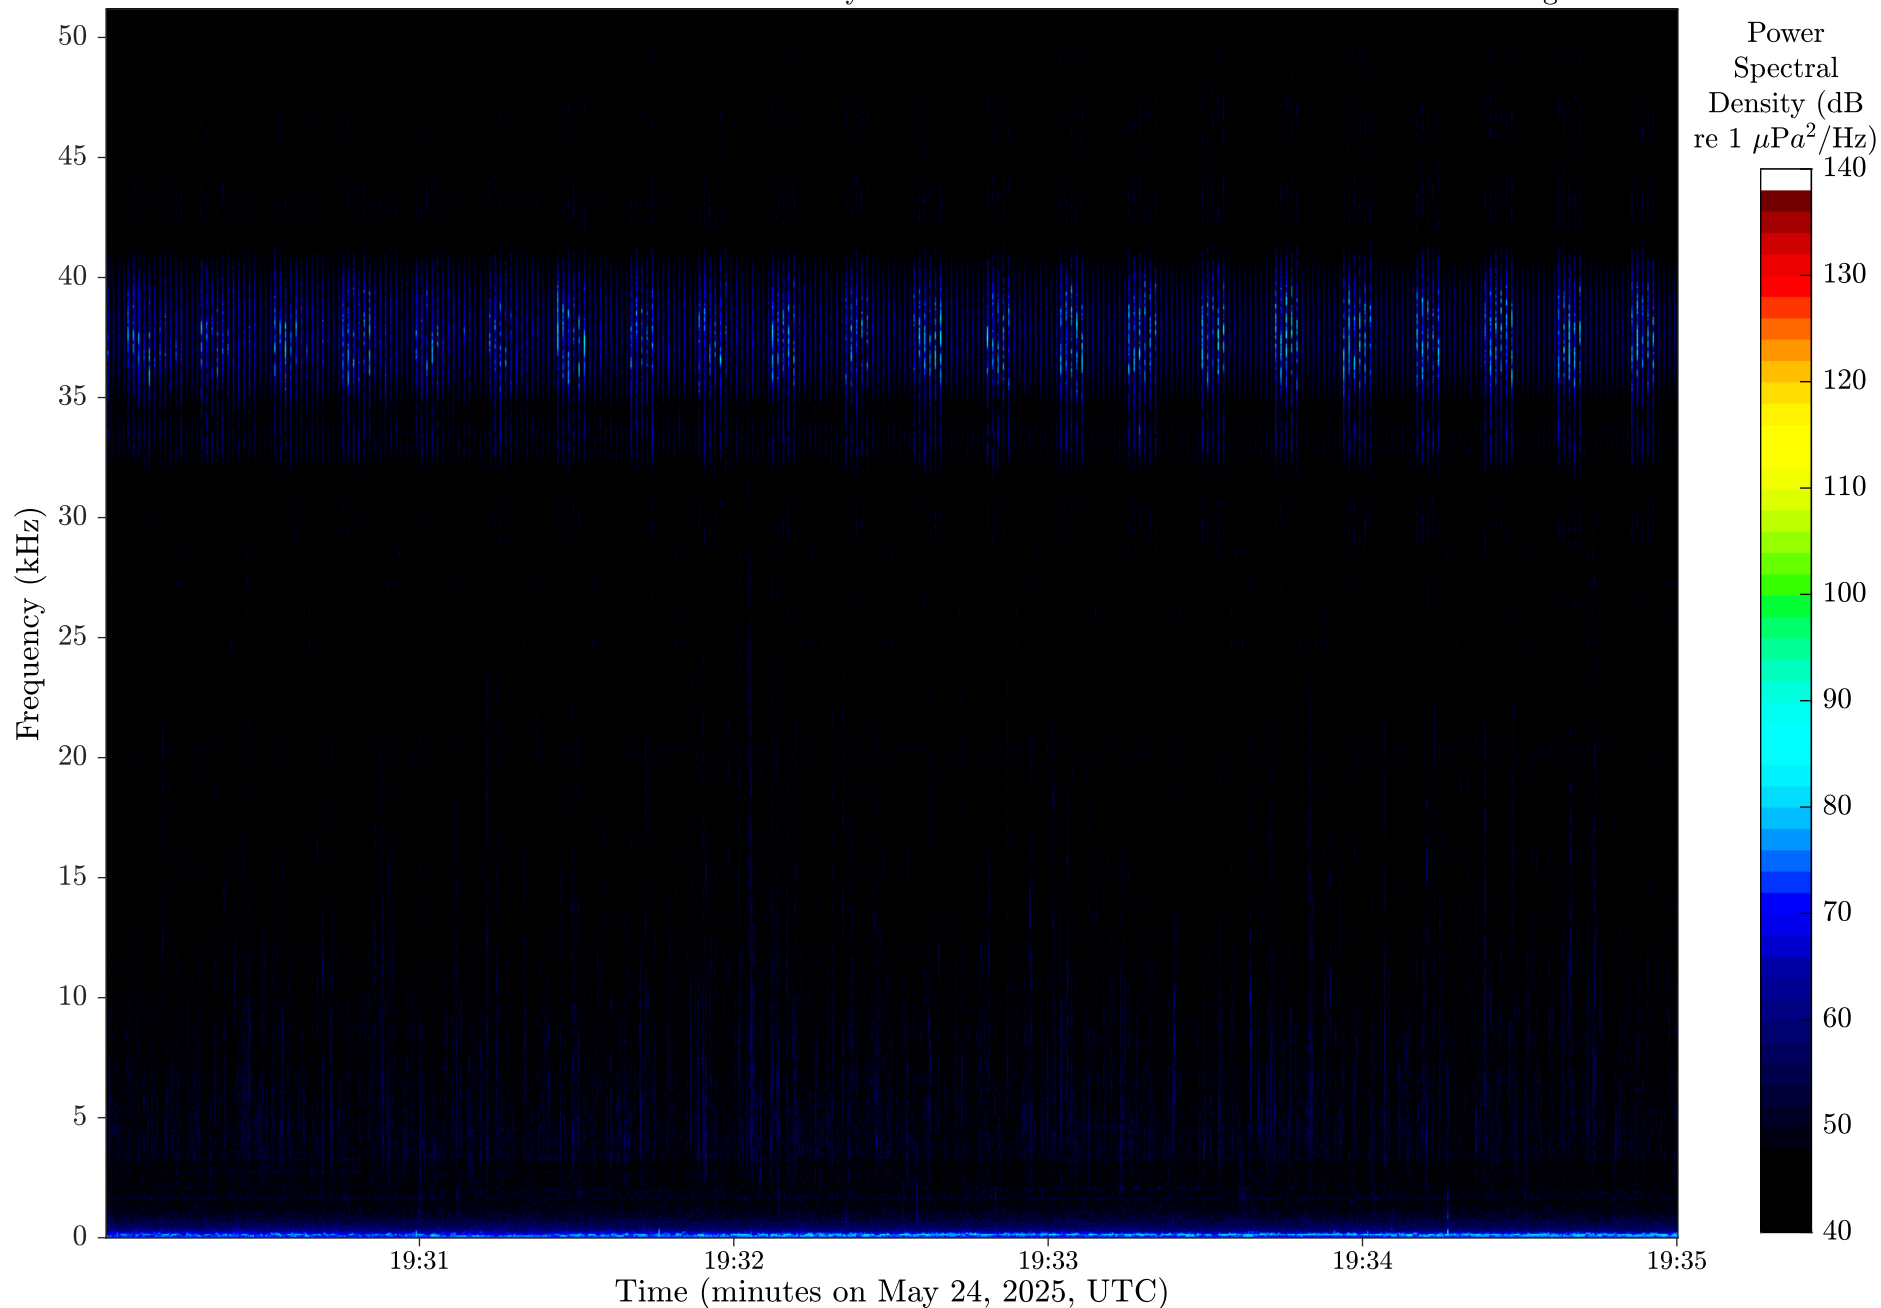


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:12 UTC

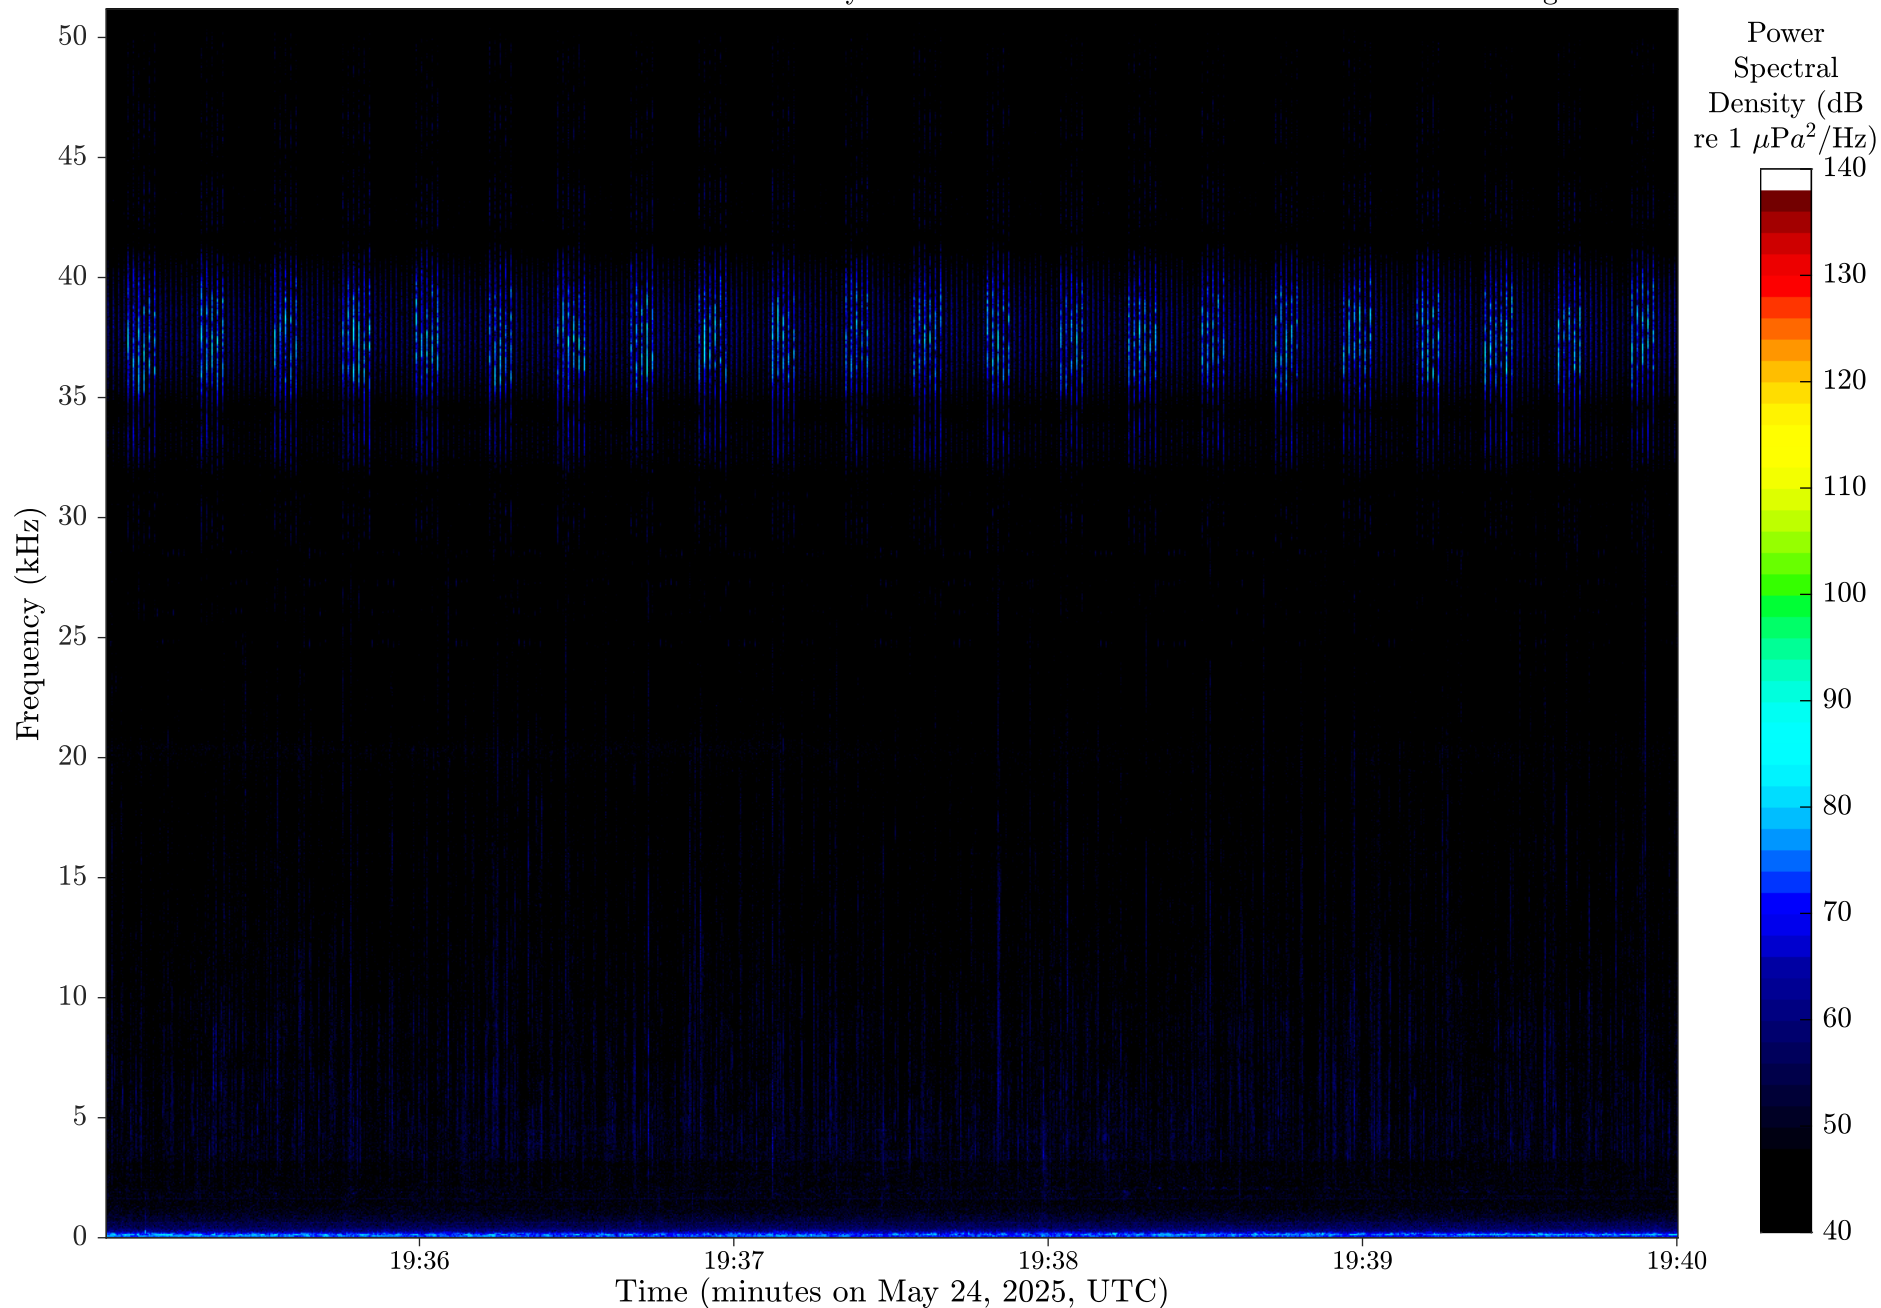


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:21 UTC

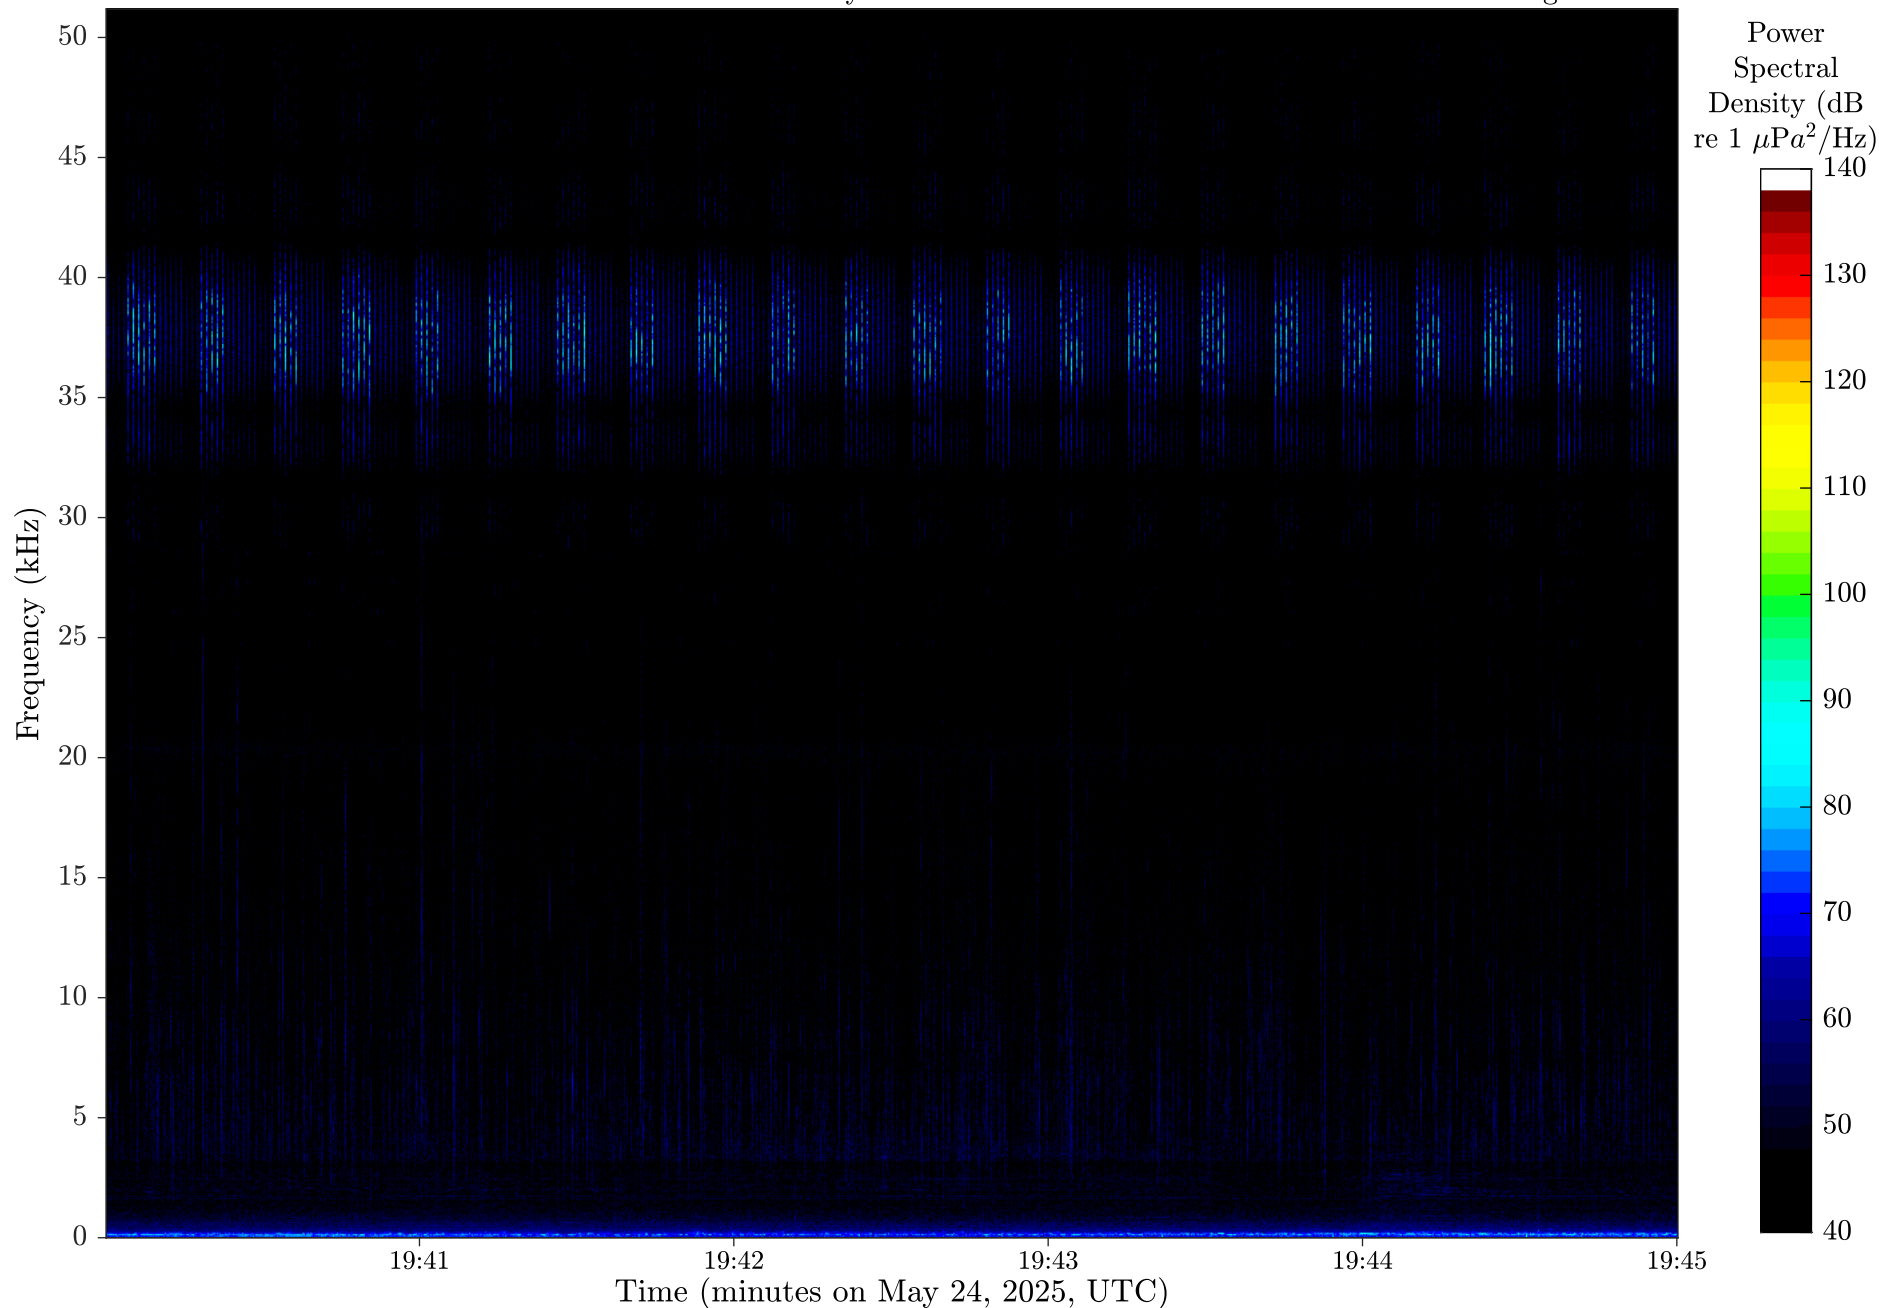


Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:30 UTC

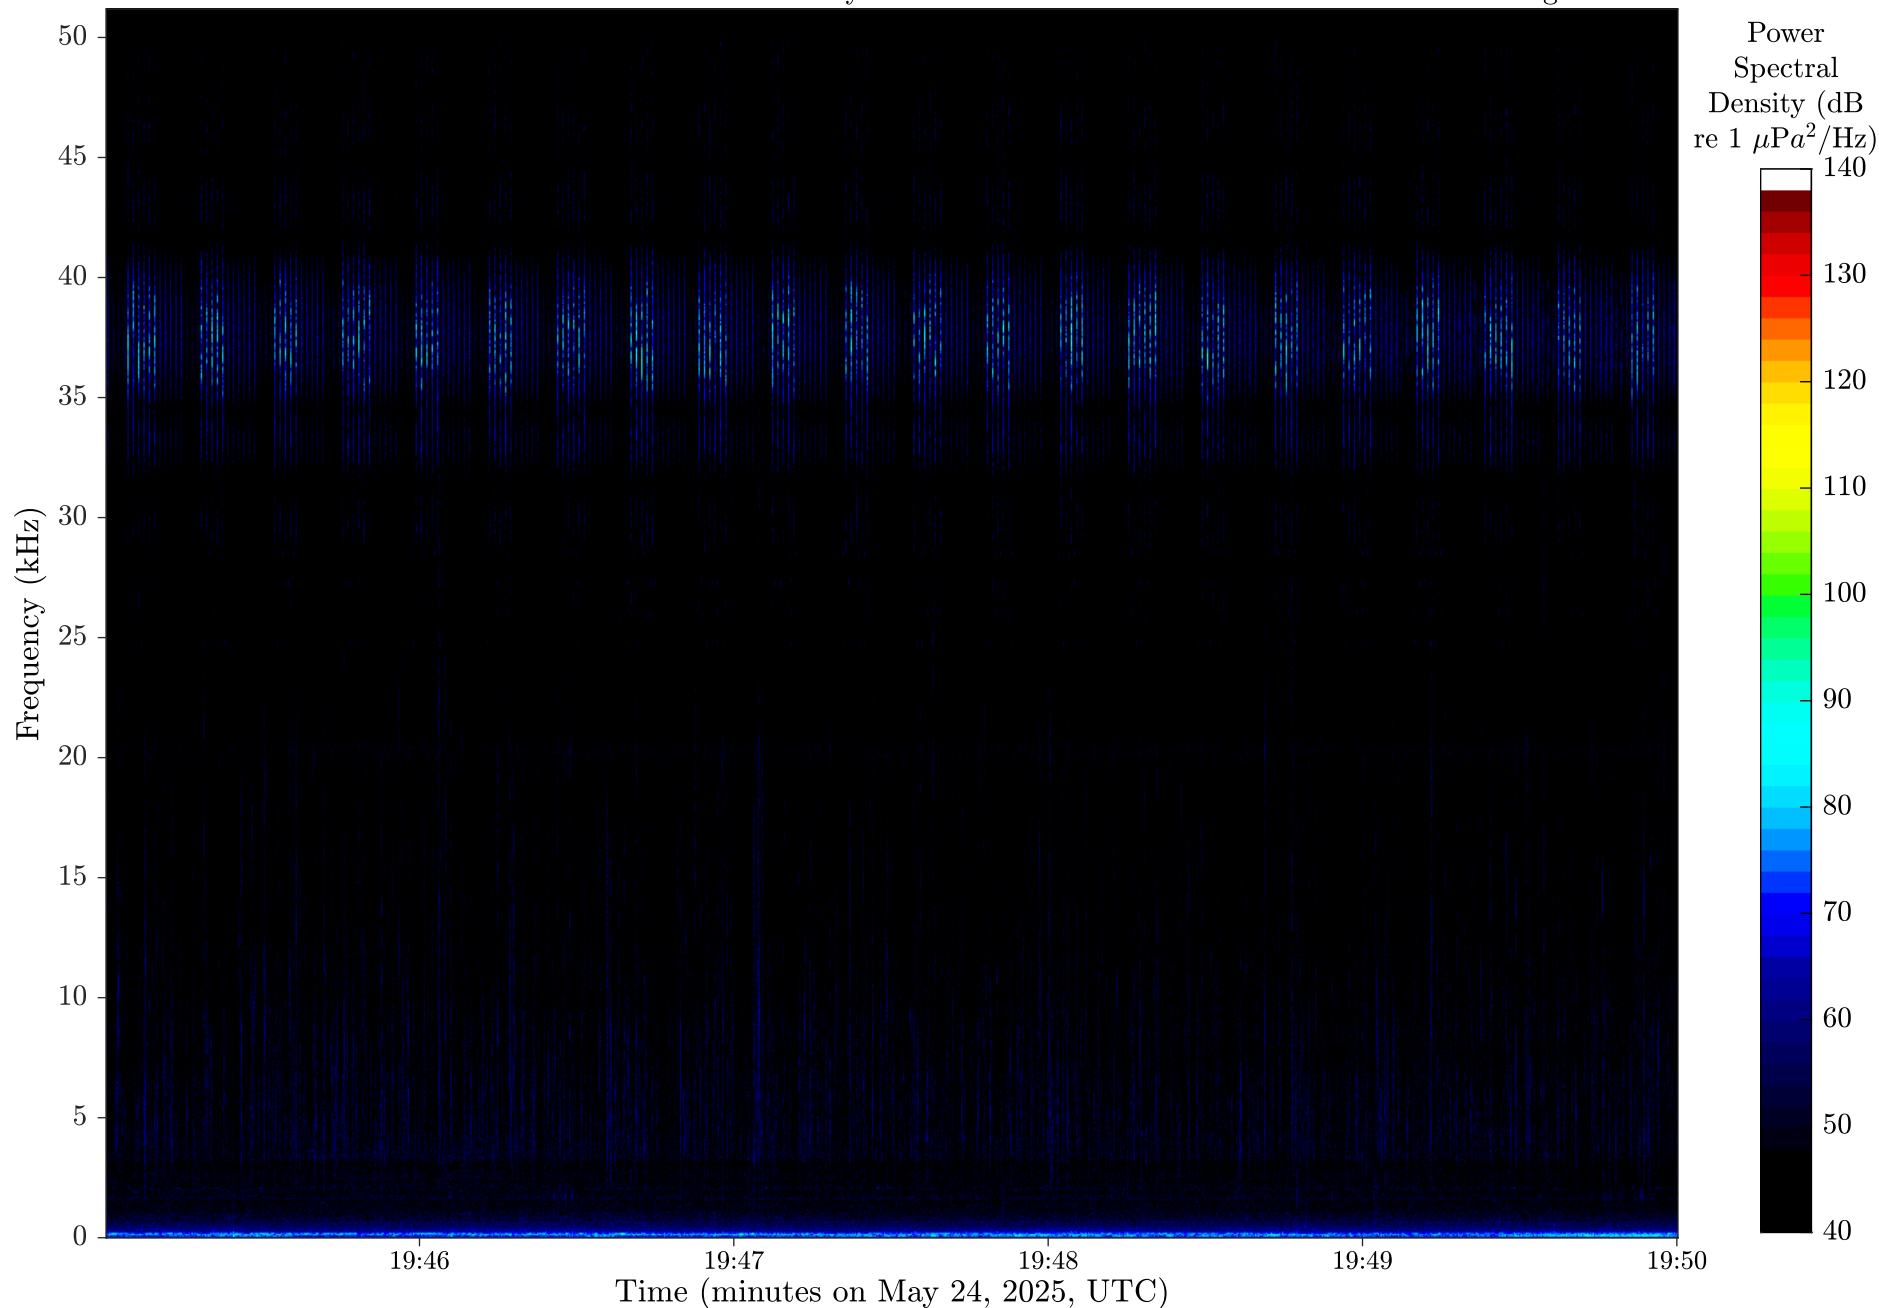


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:38 UTC

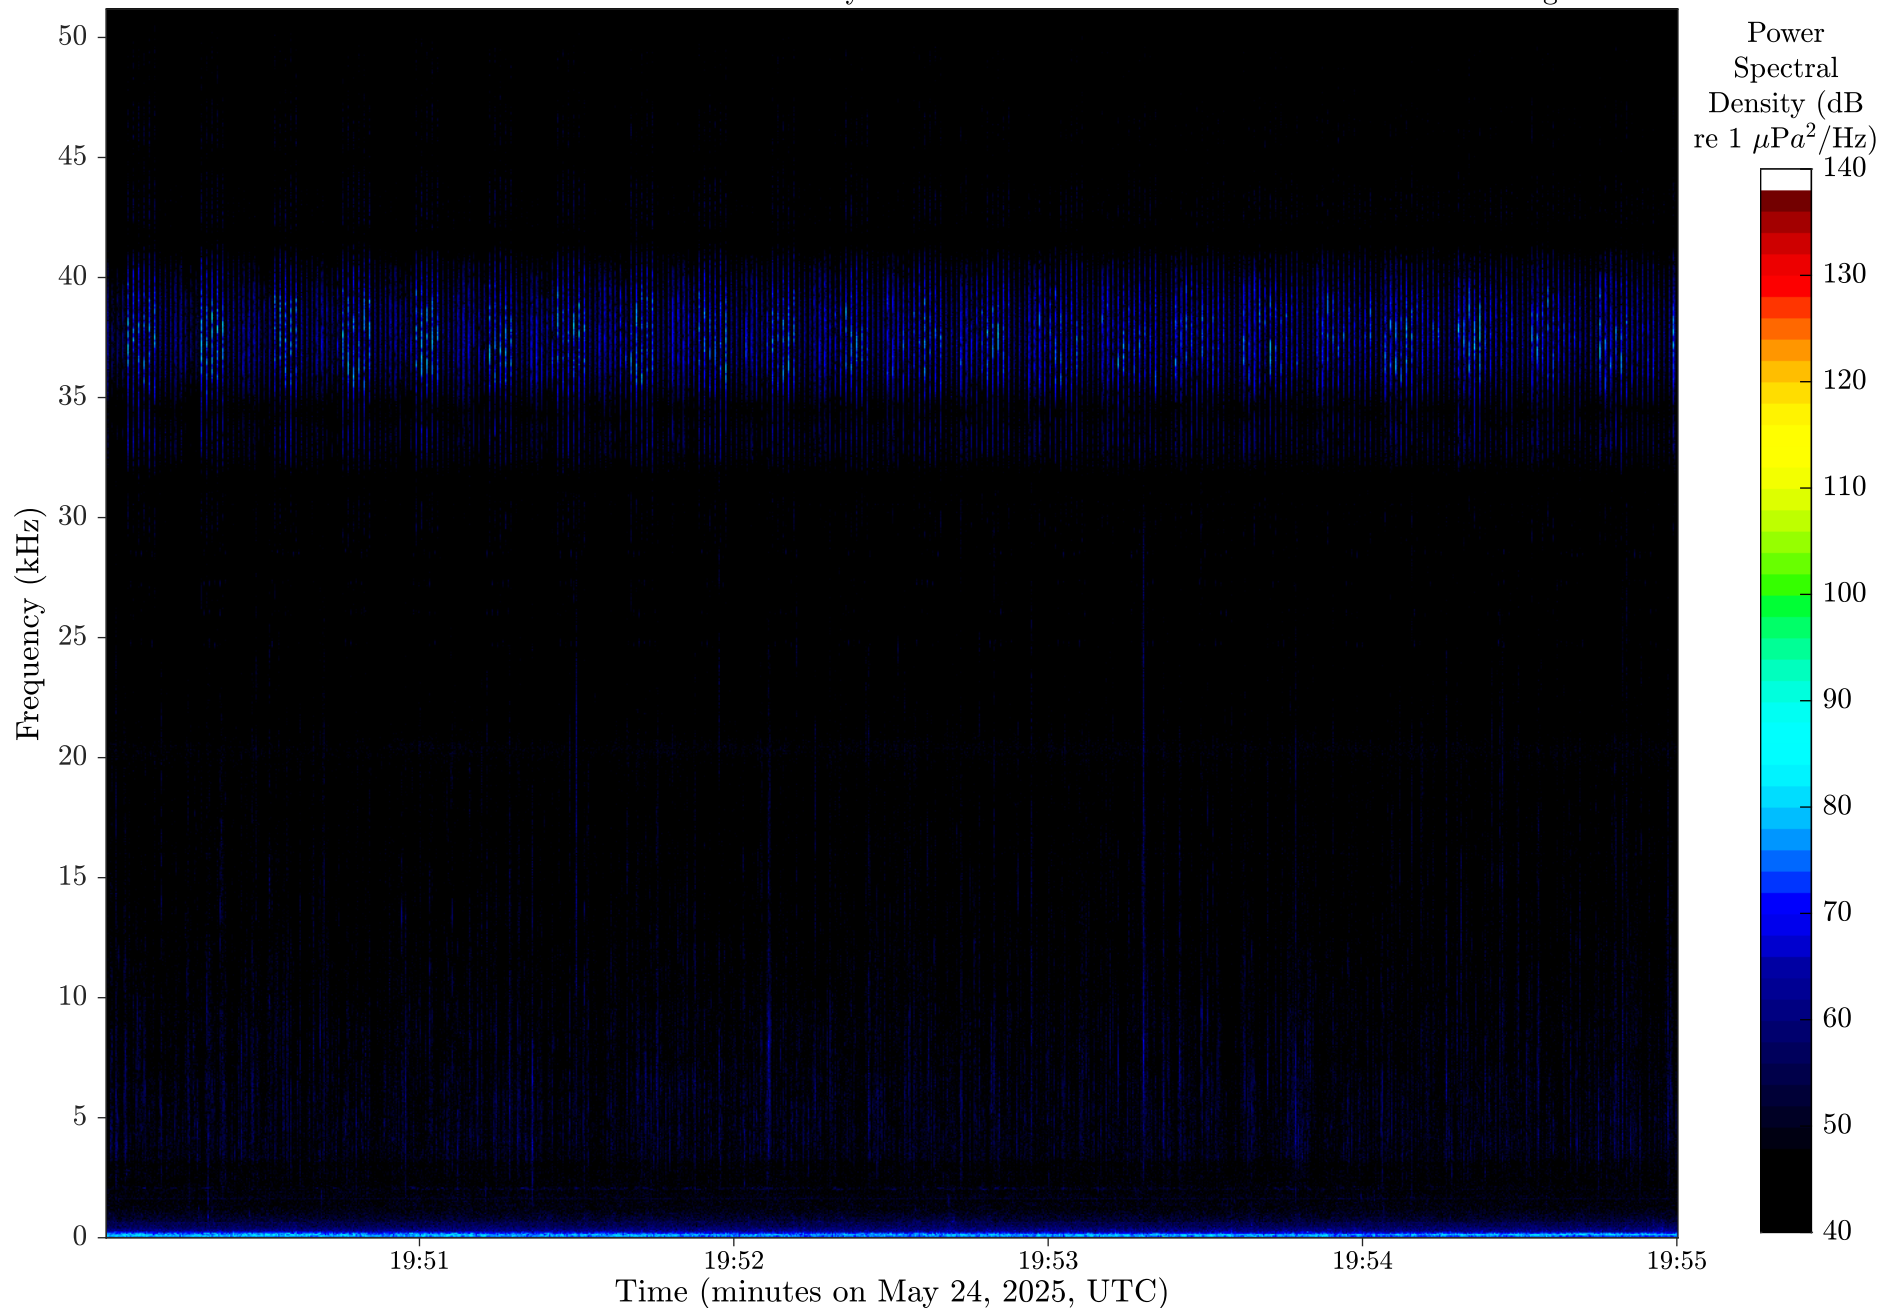


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:45 UTC

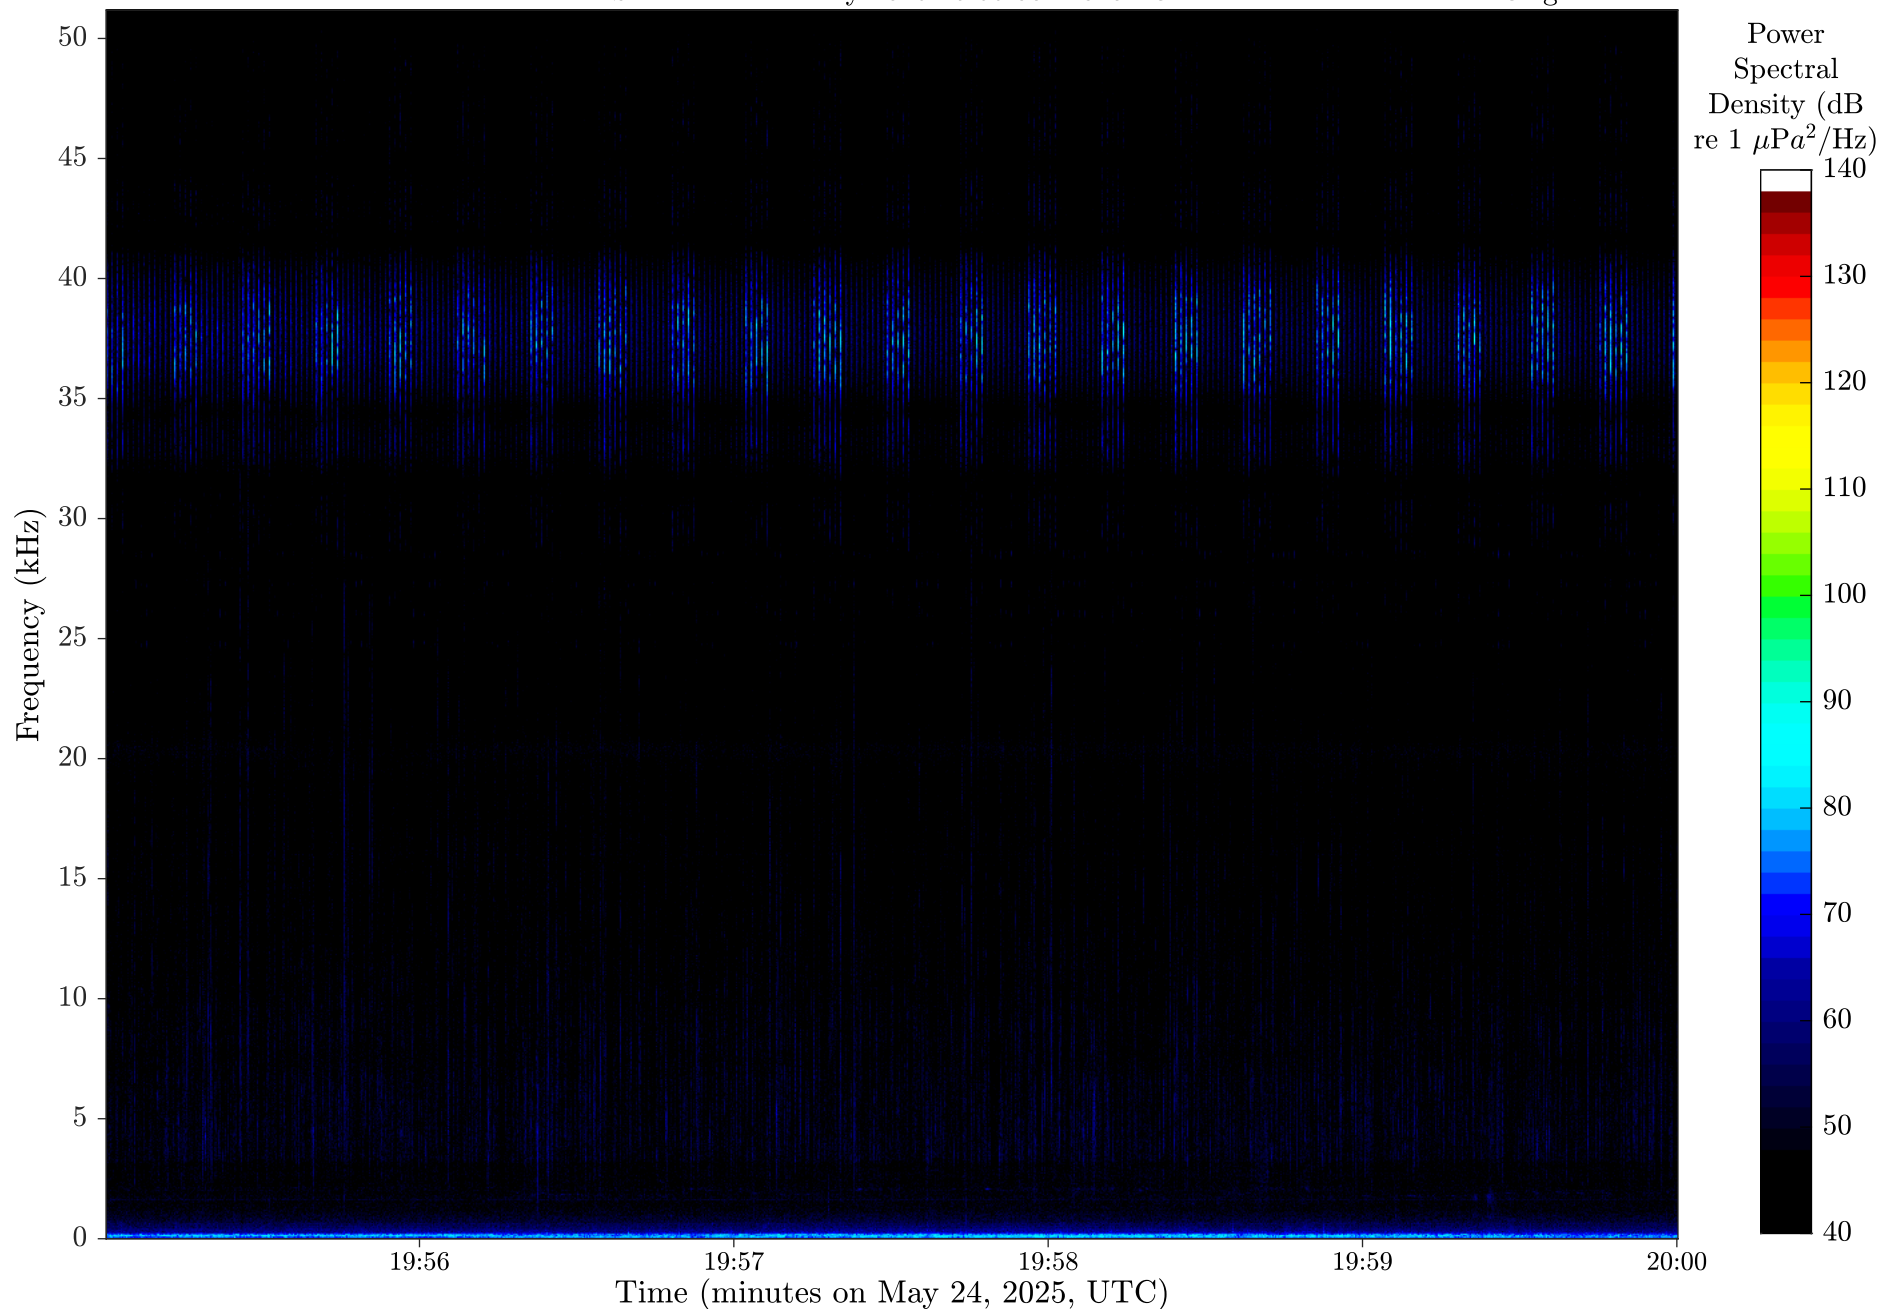


Comments: 34.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:53 UTC

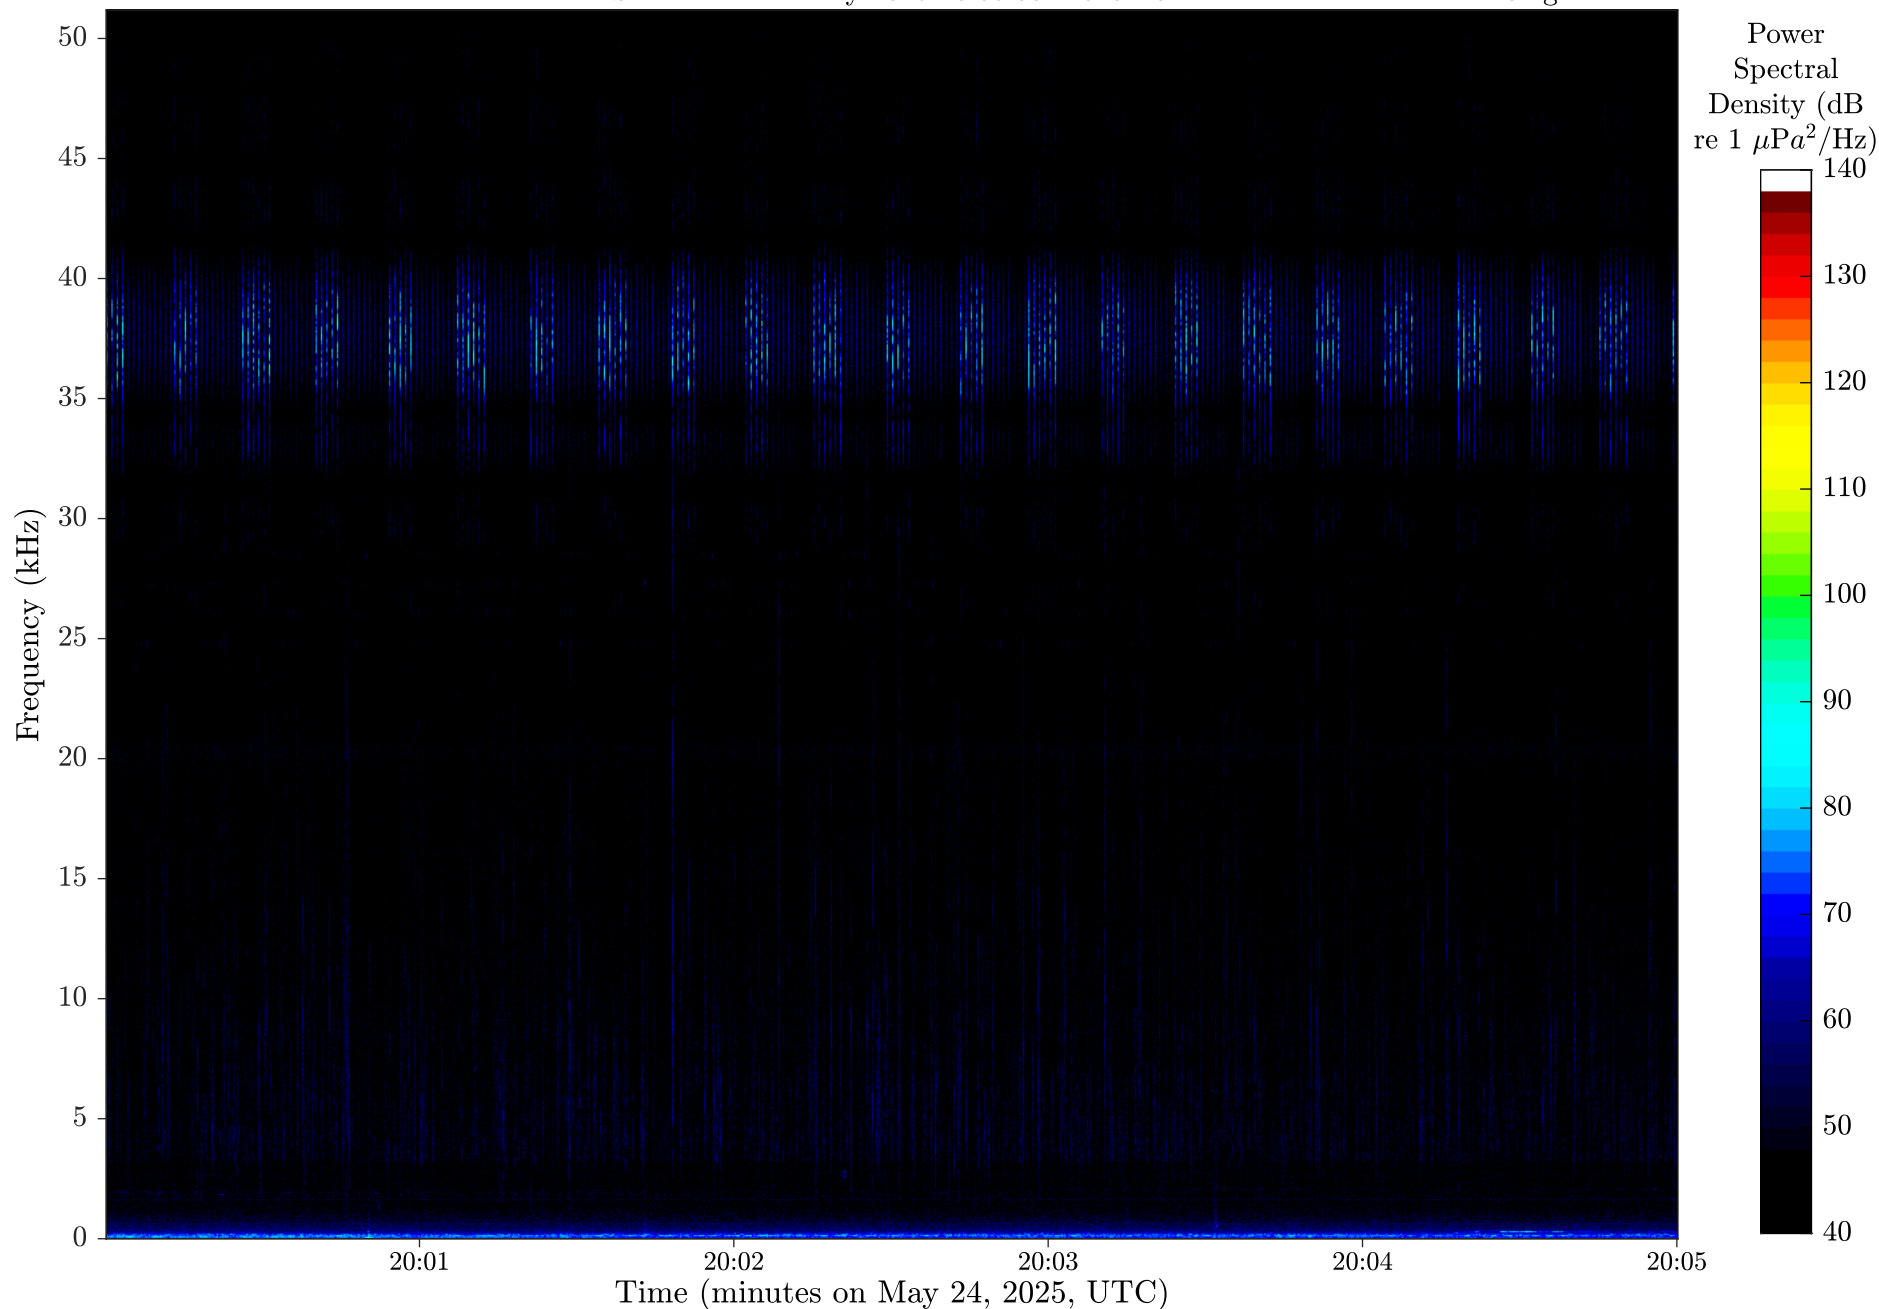


Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:01 UTC

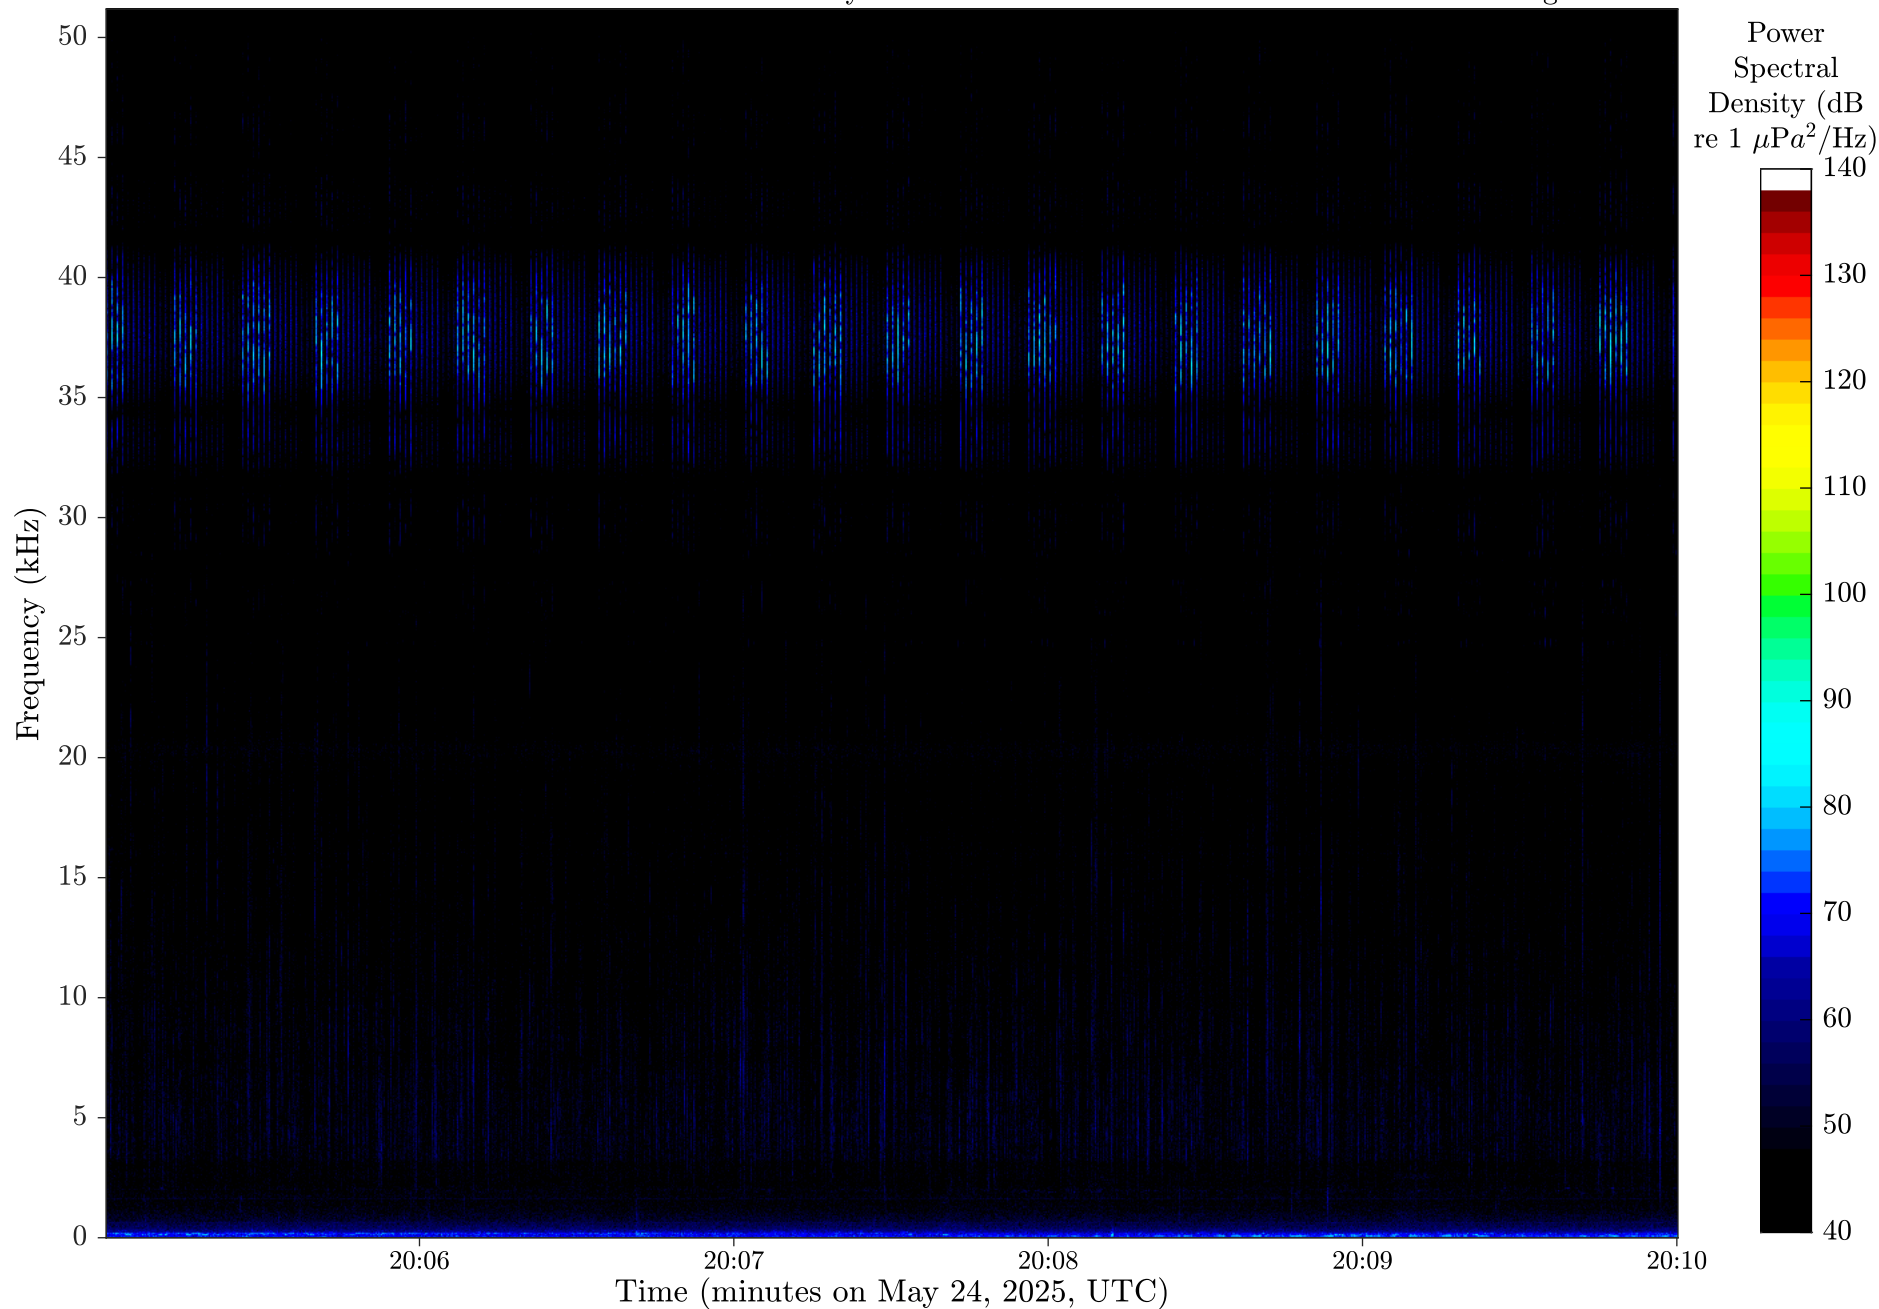


Comments: 35.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:40:09 UTC

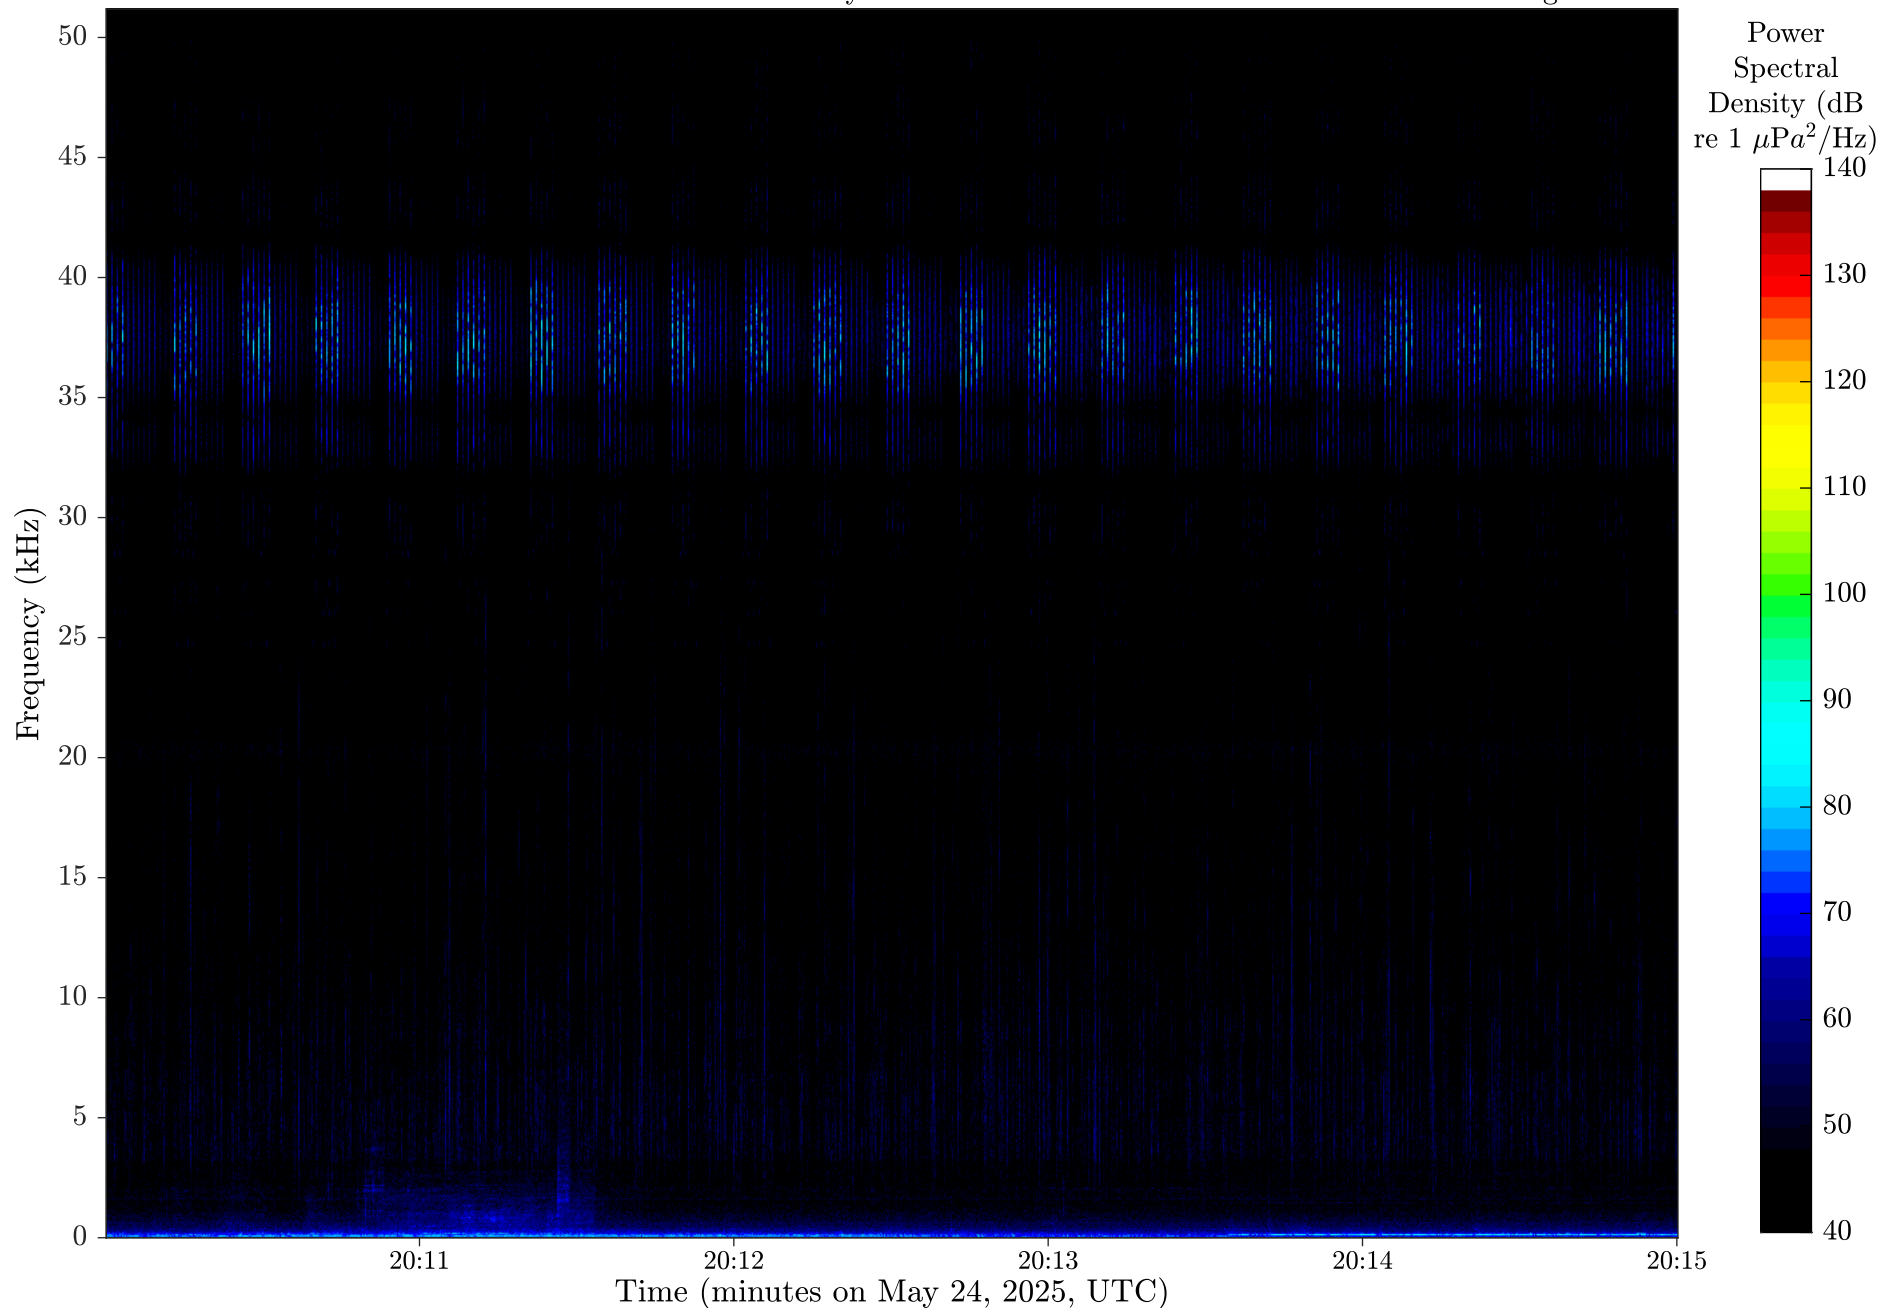

Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:40:17 UTC

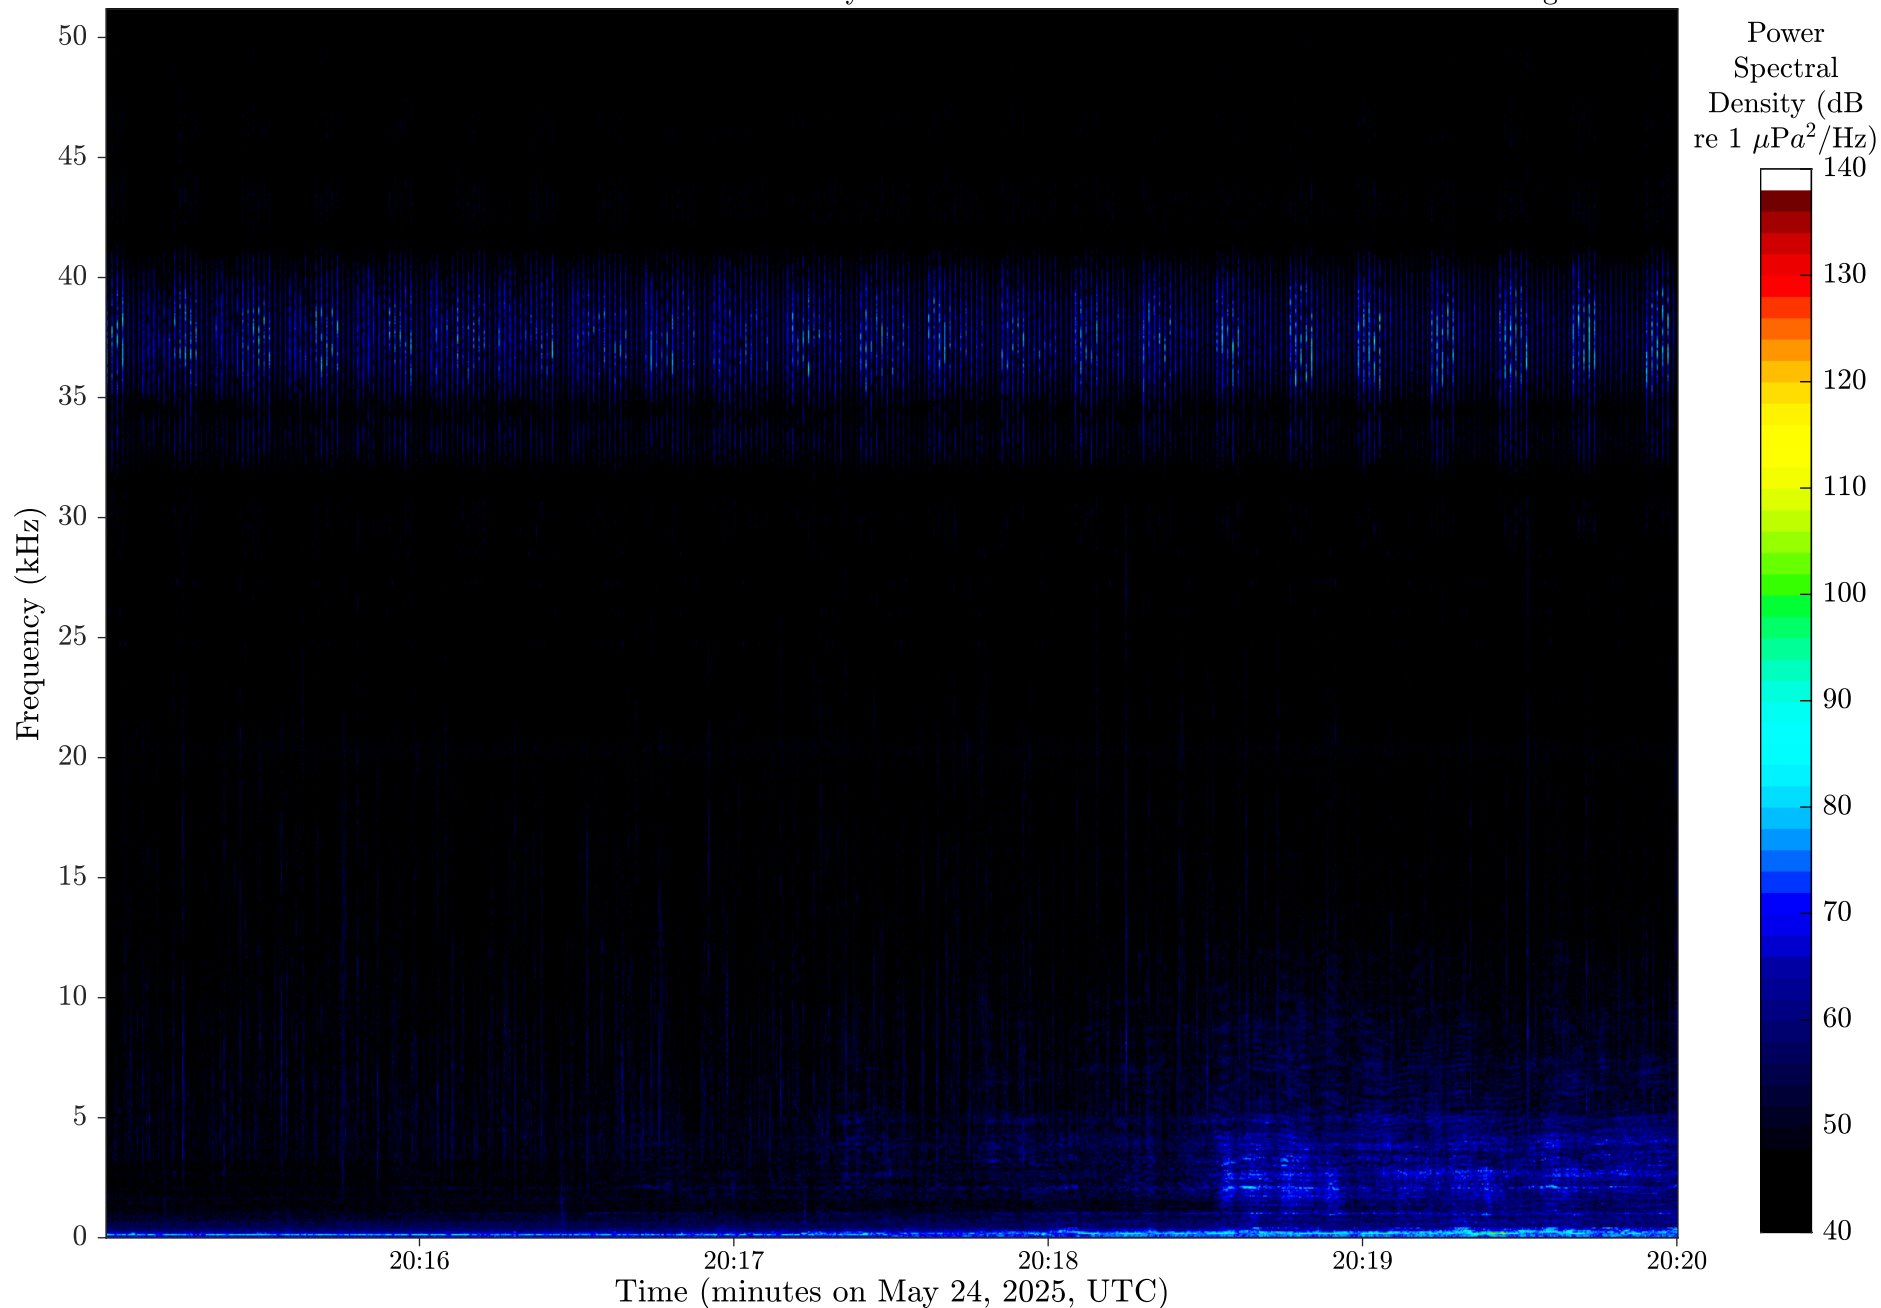

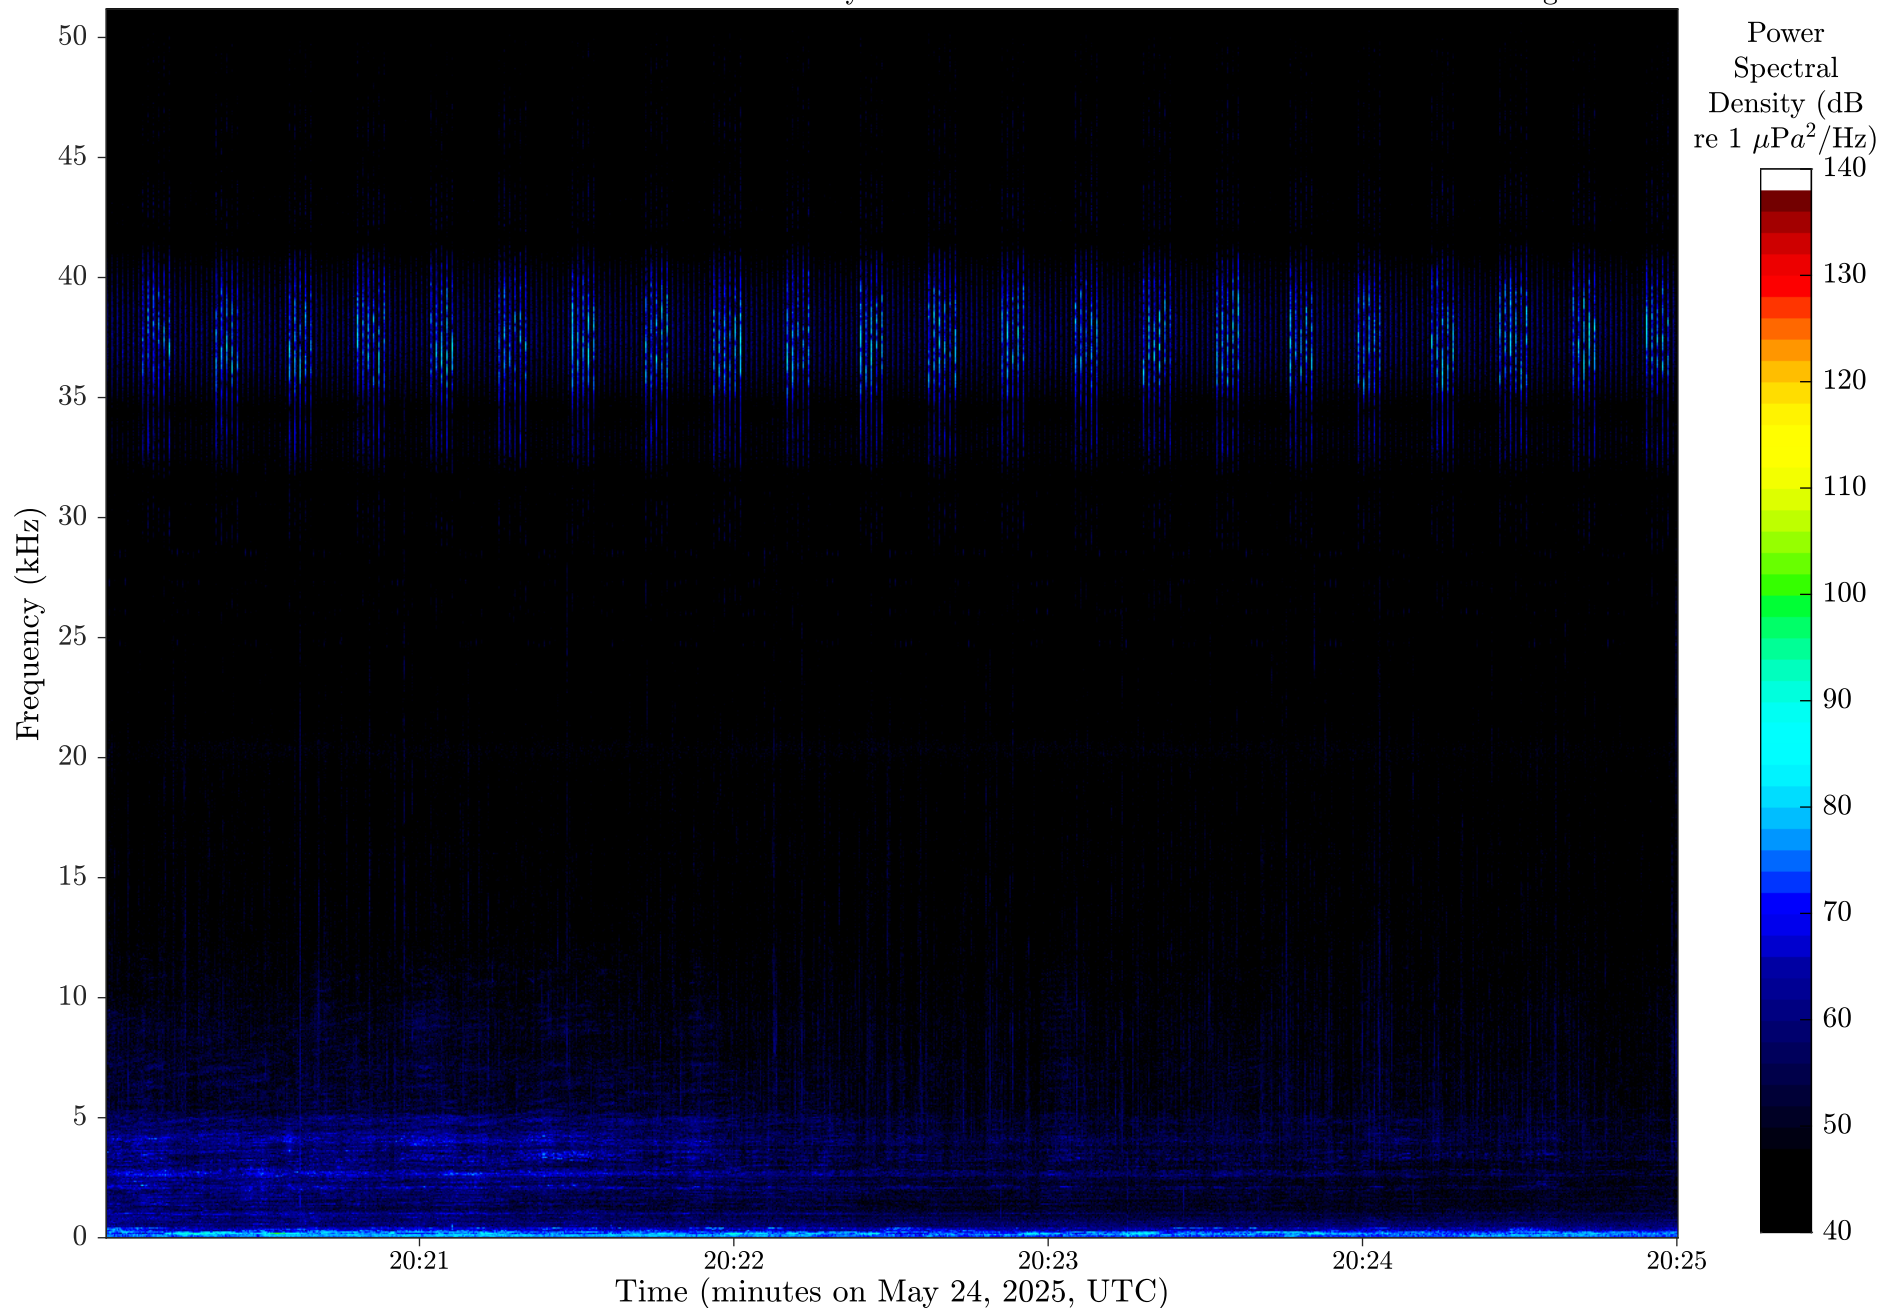


Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:34 UTC

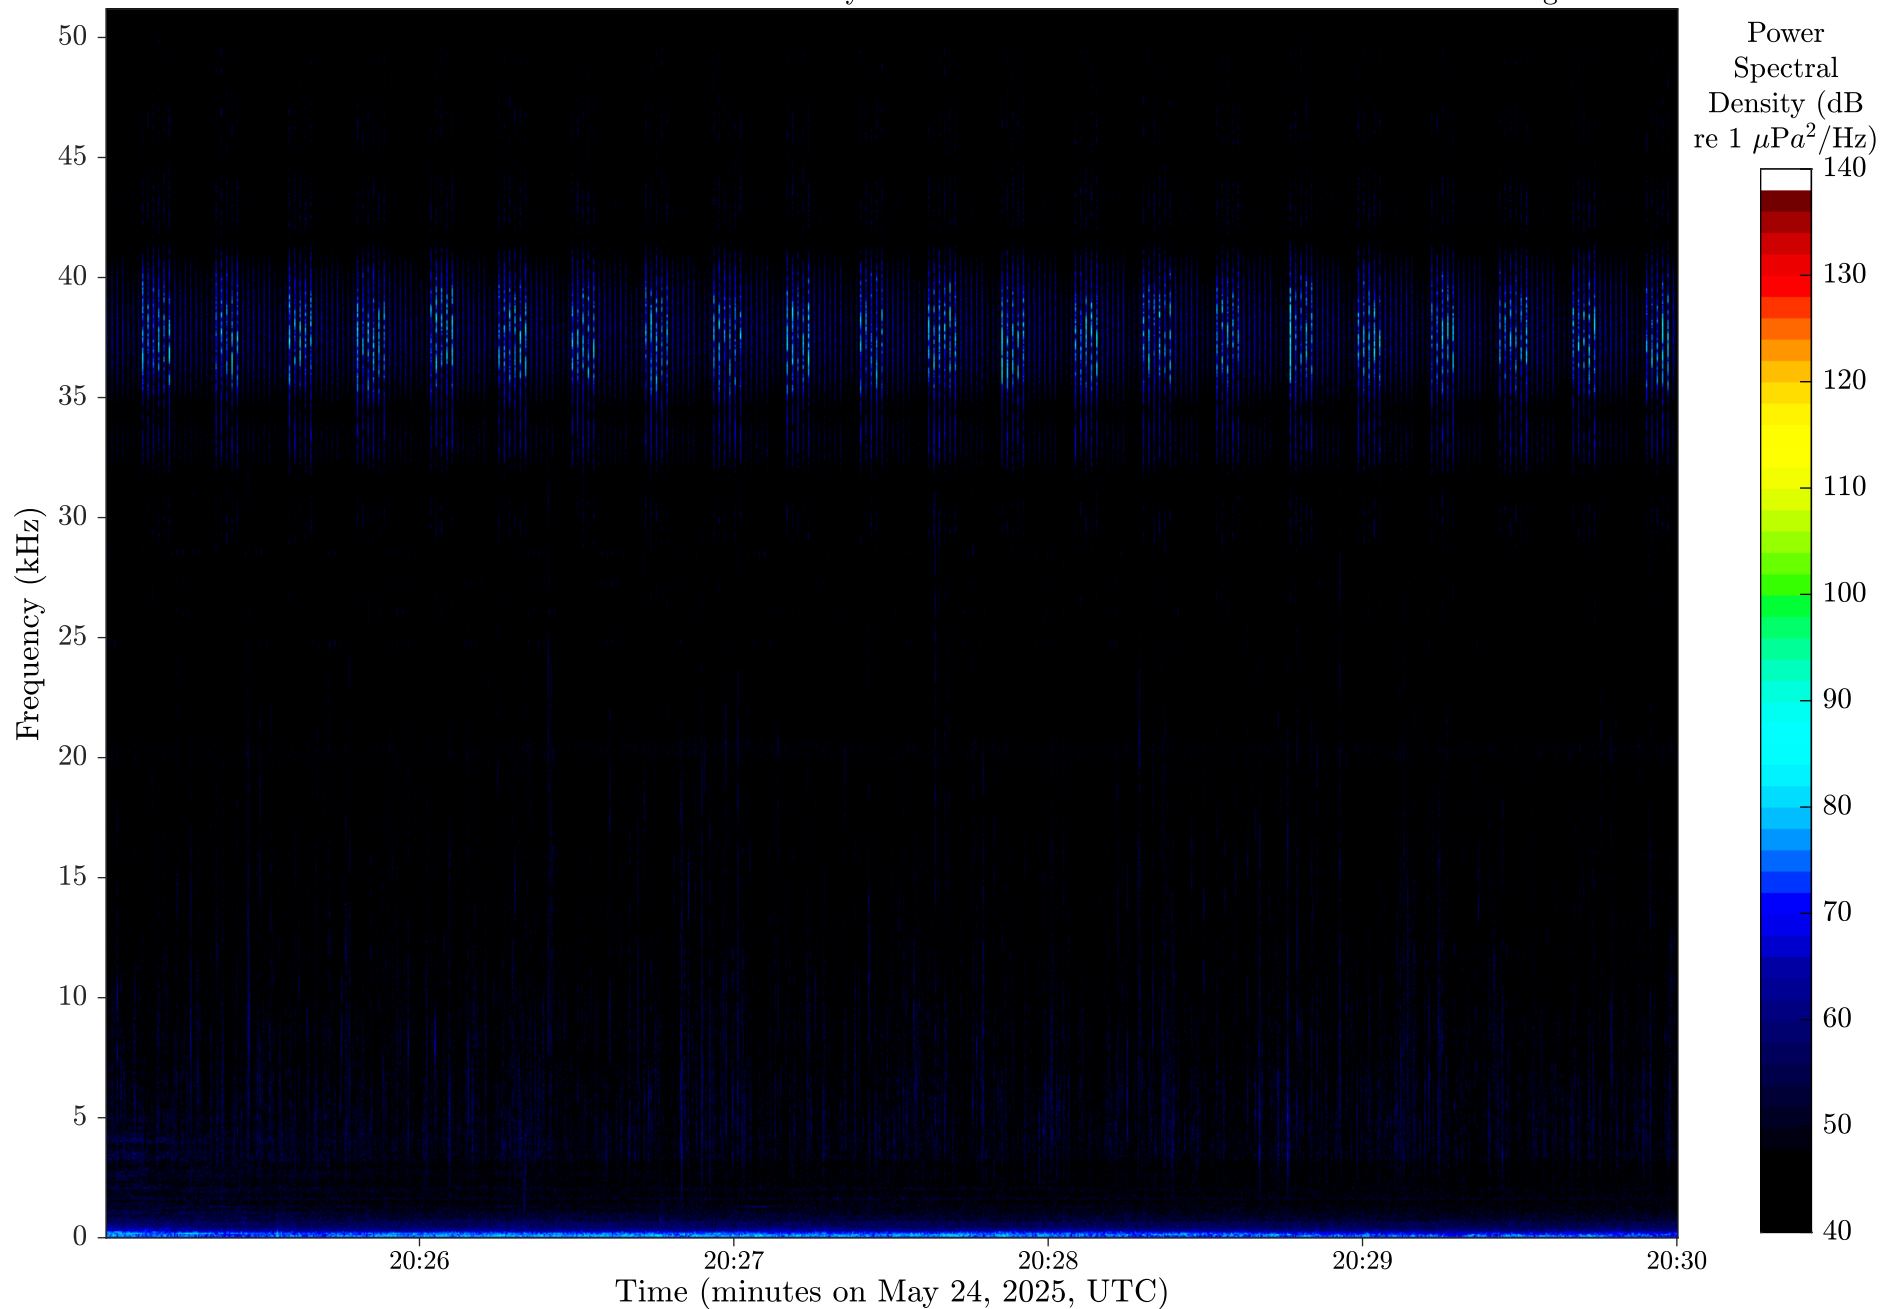


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:42 UTC

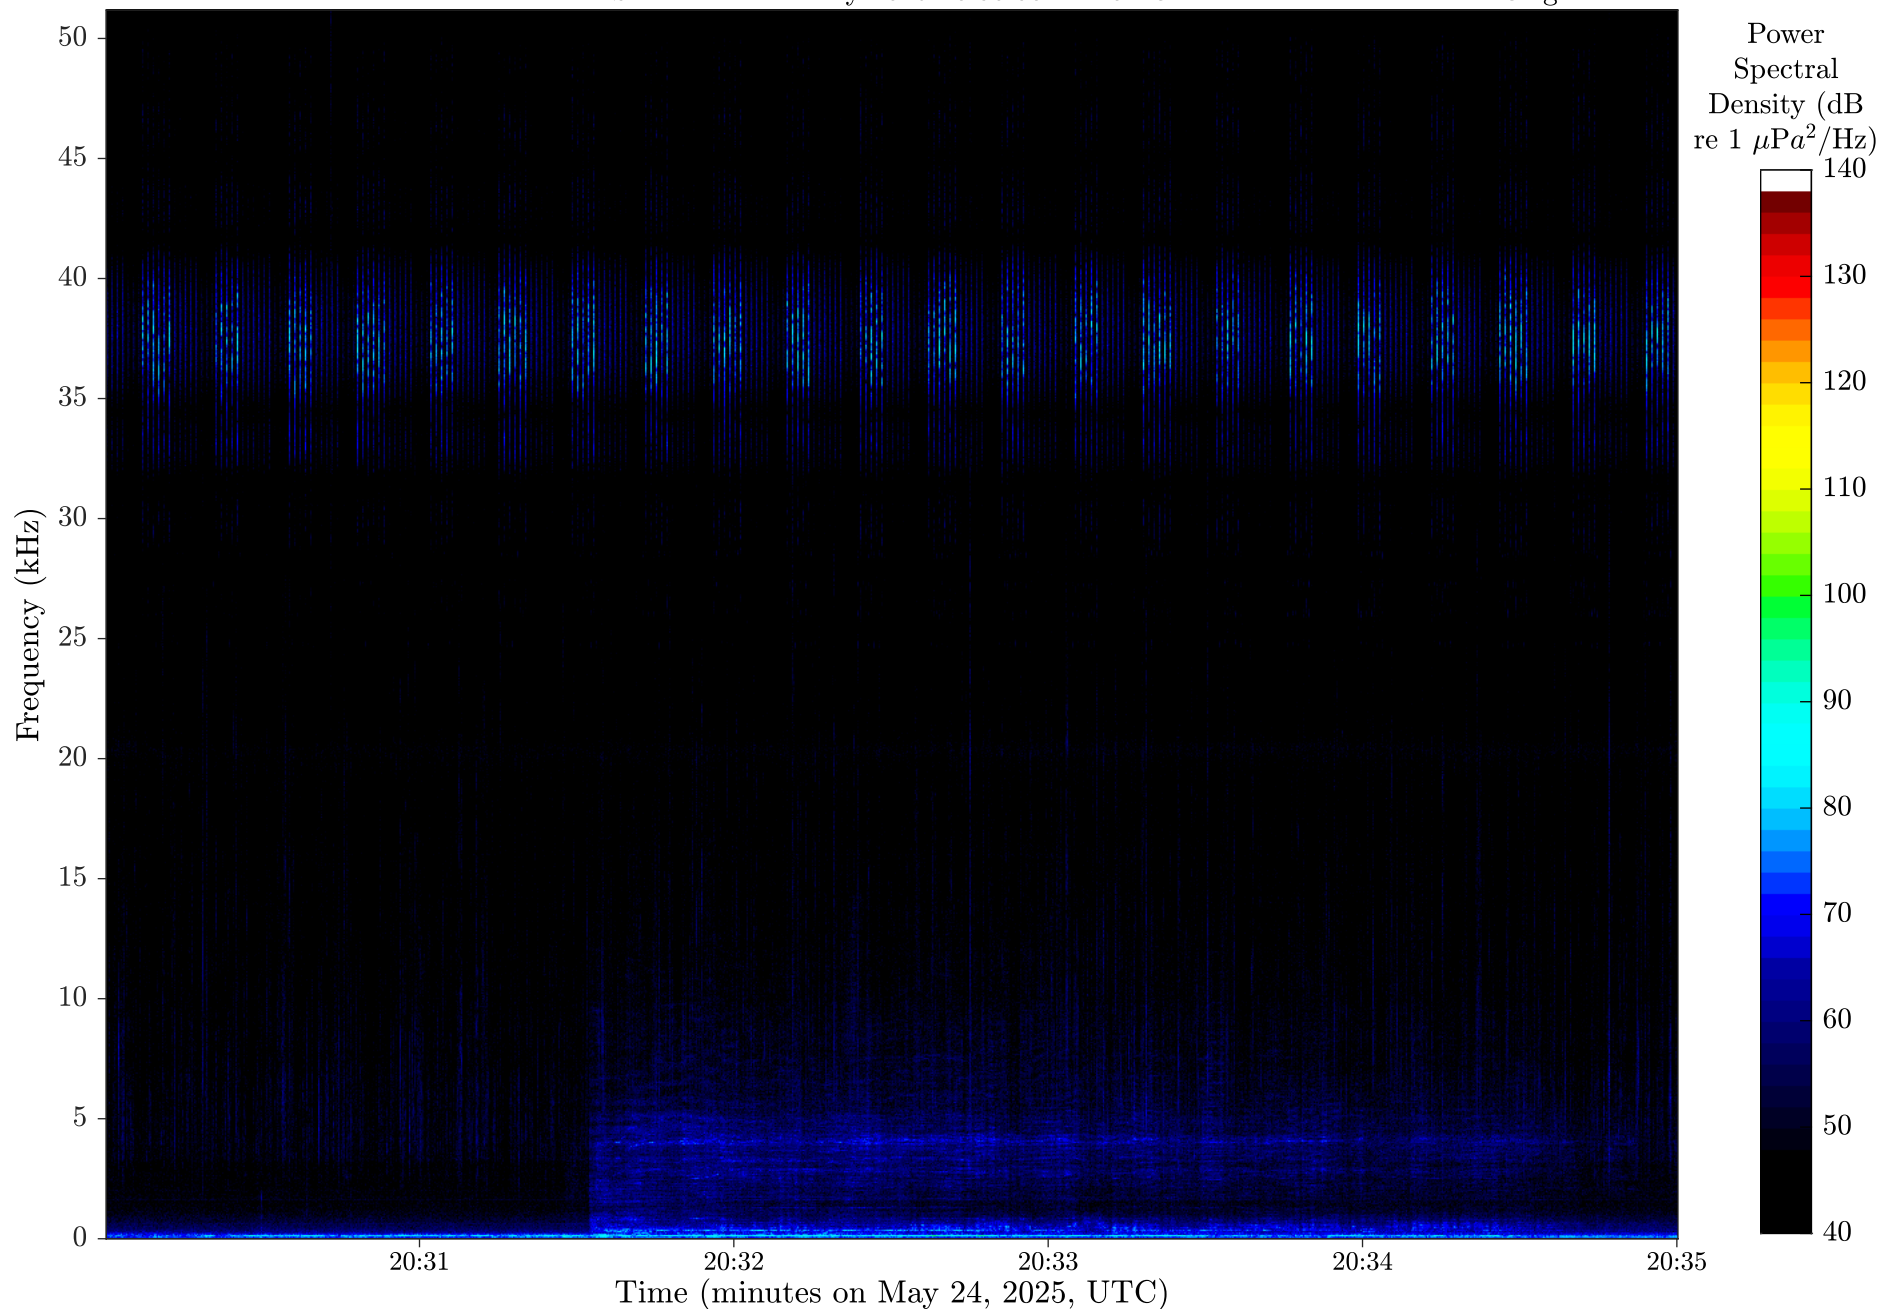


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:50 UTC

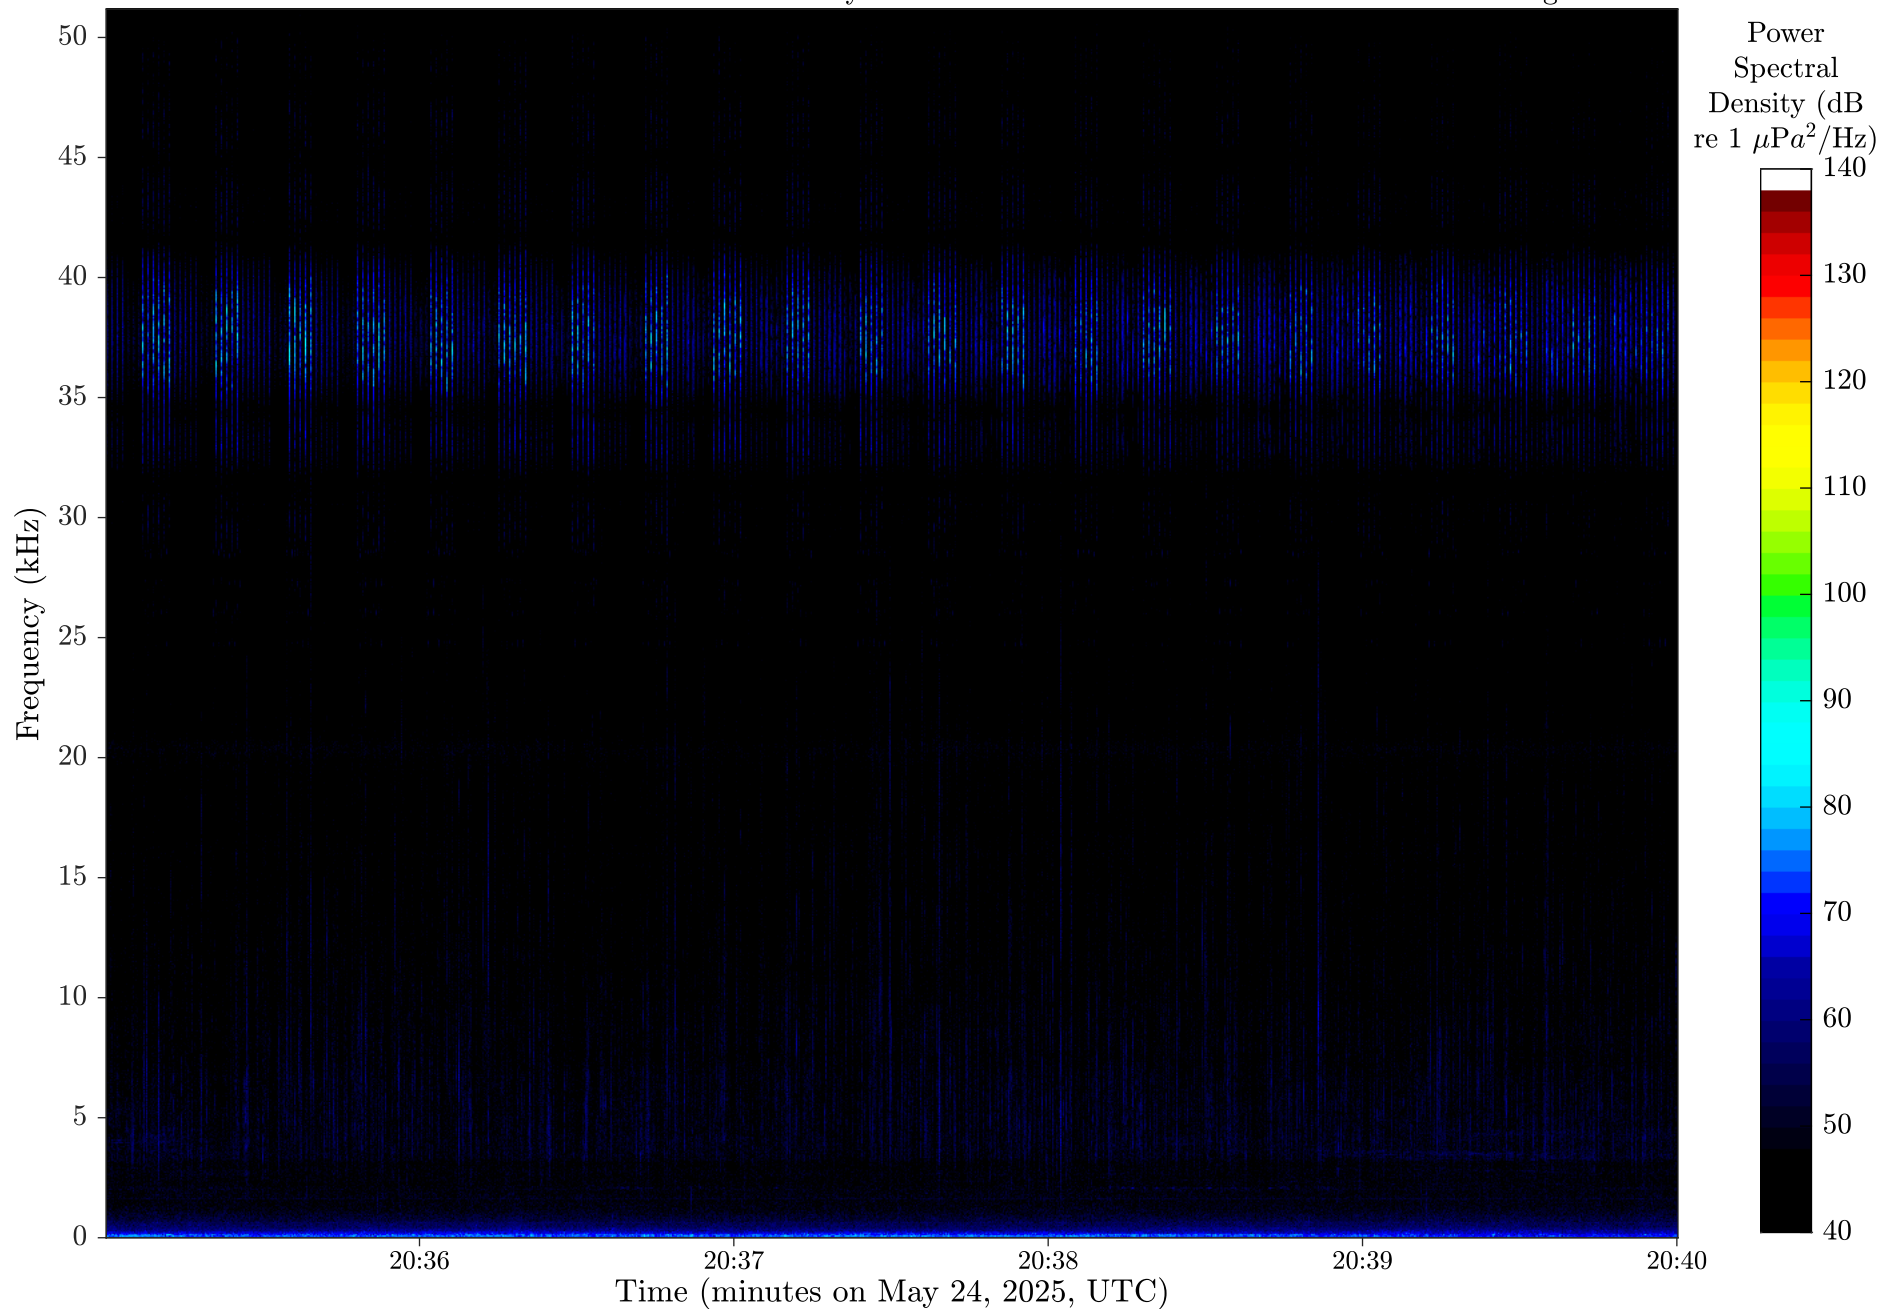


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:58 UTC

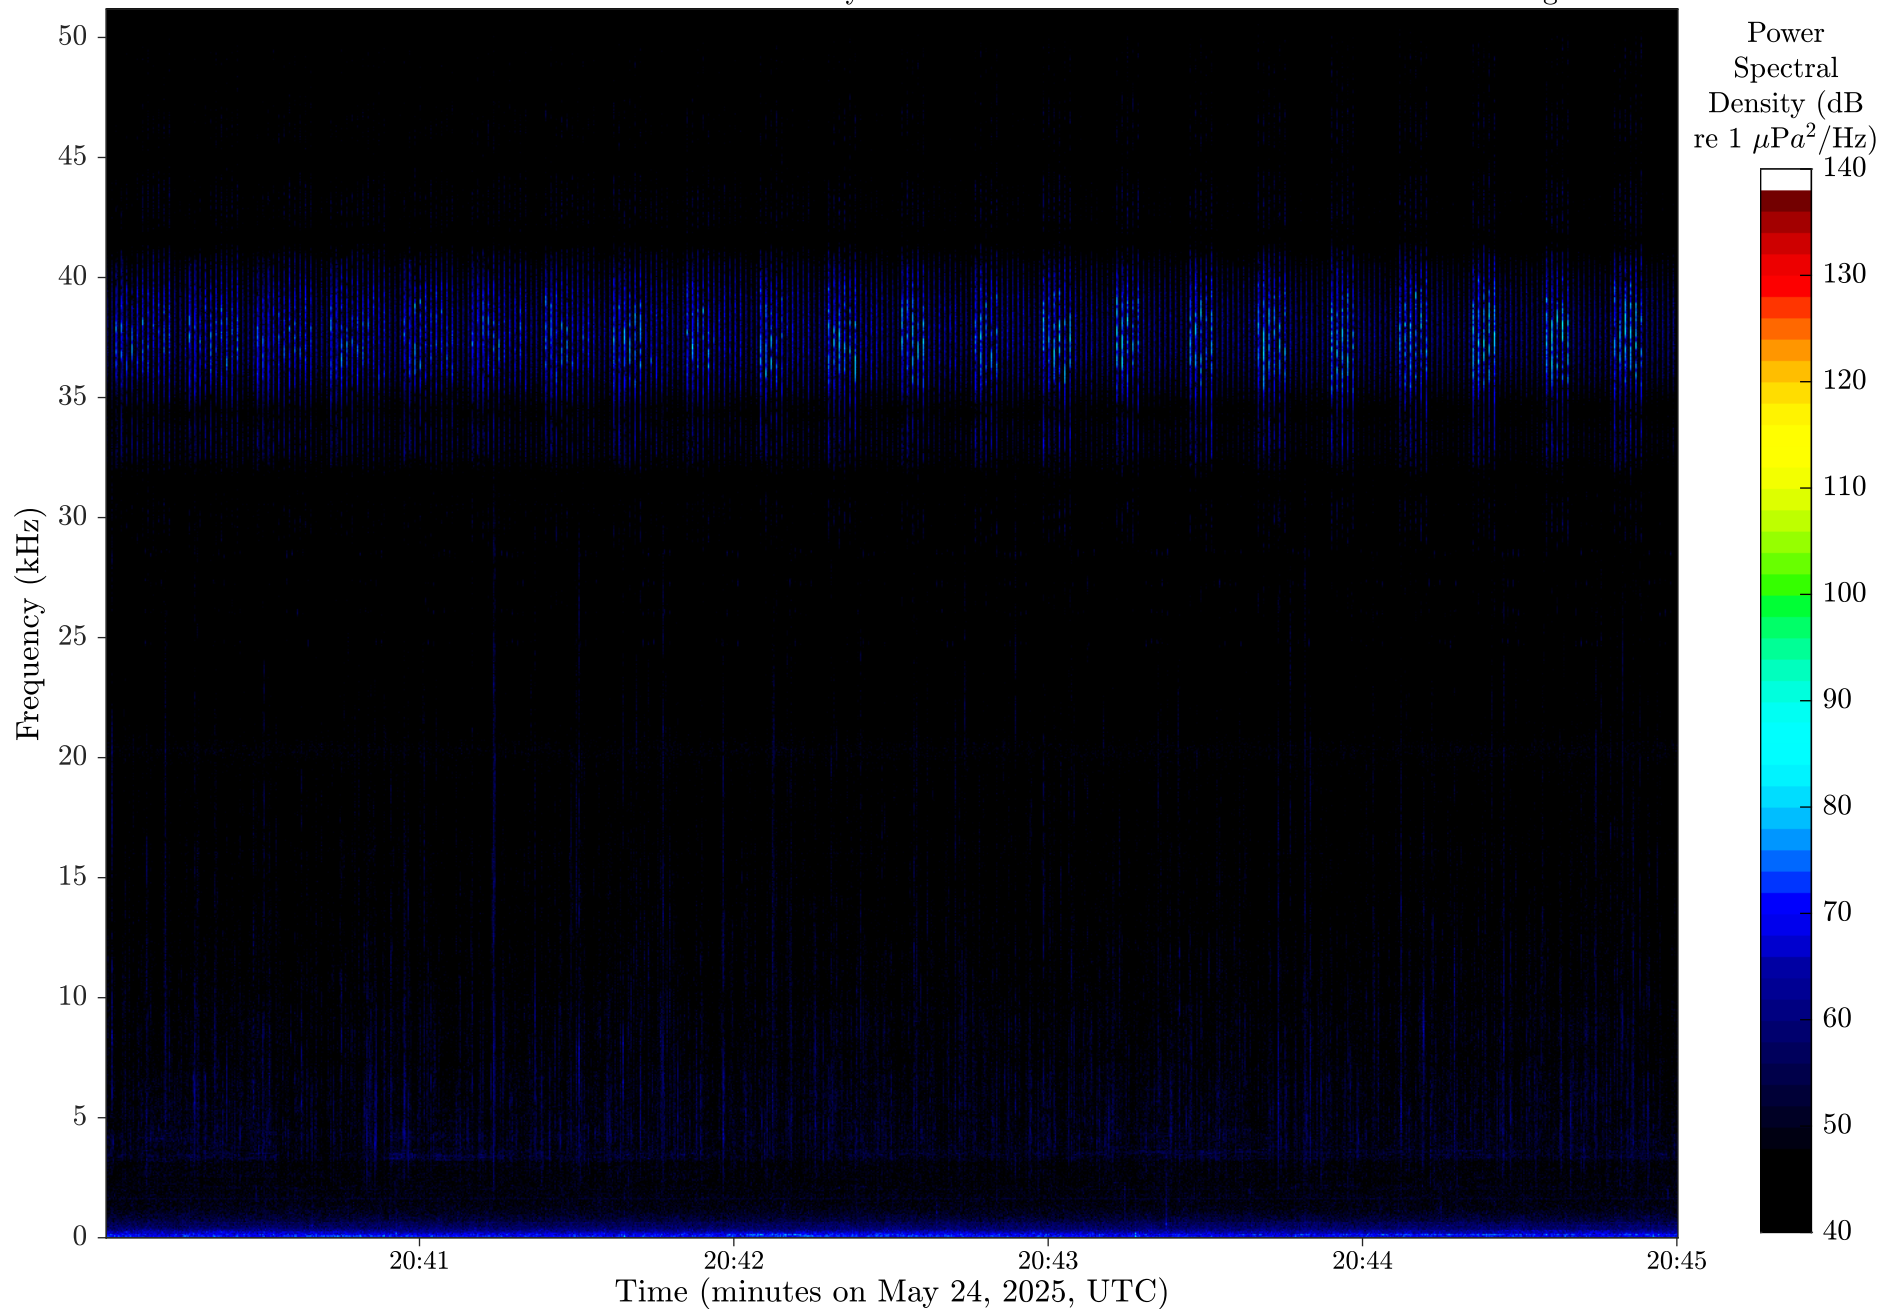


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:06 UTC

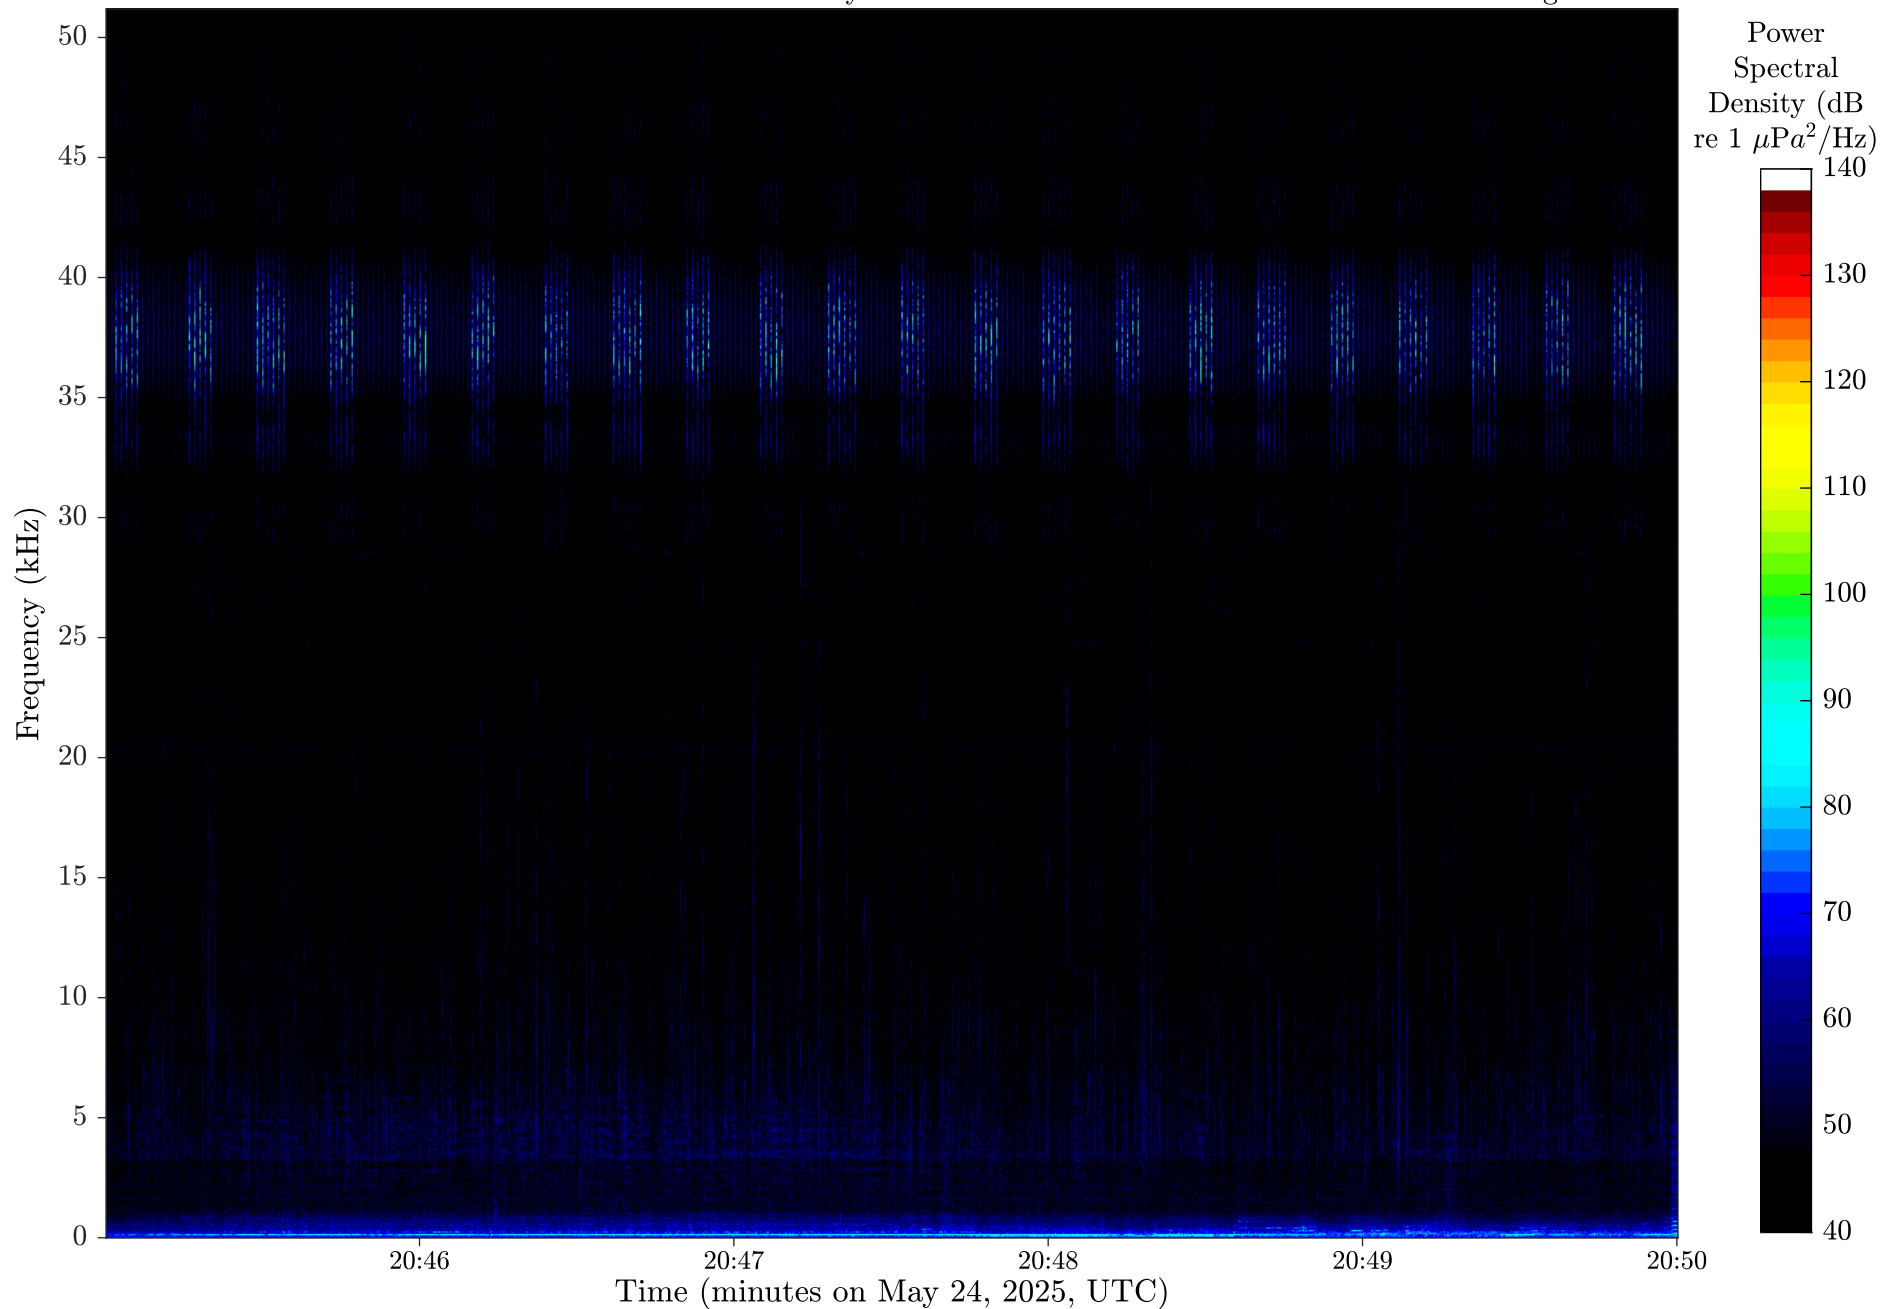


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:41:15 UTC

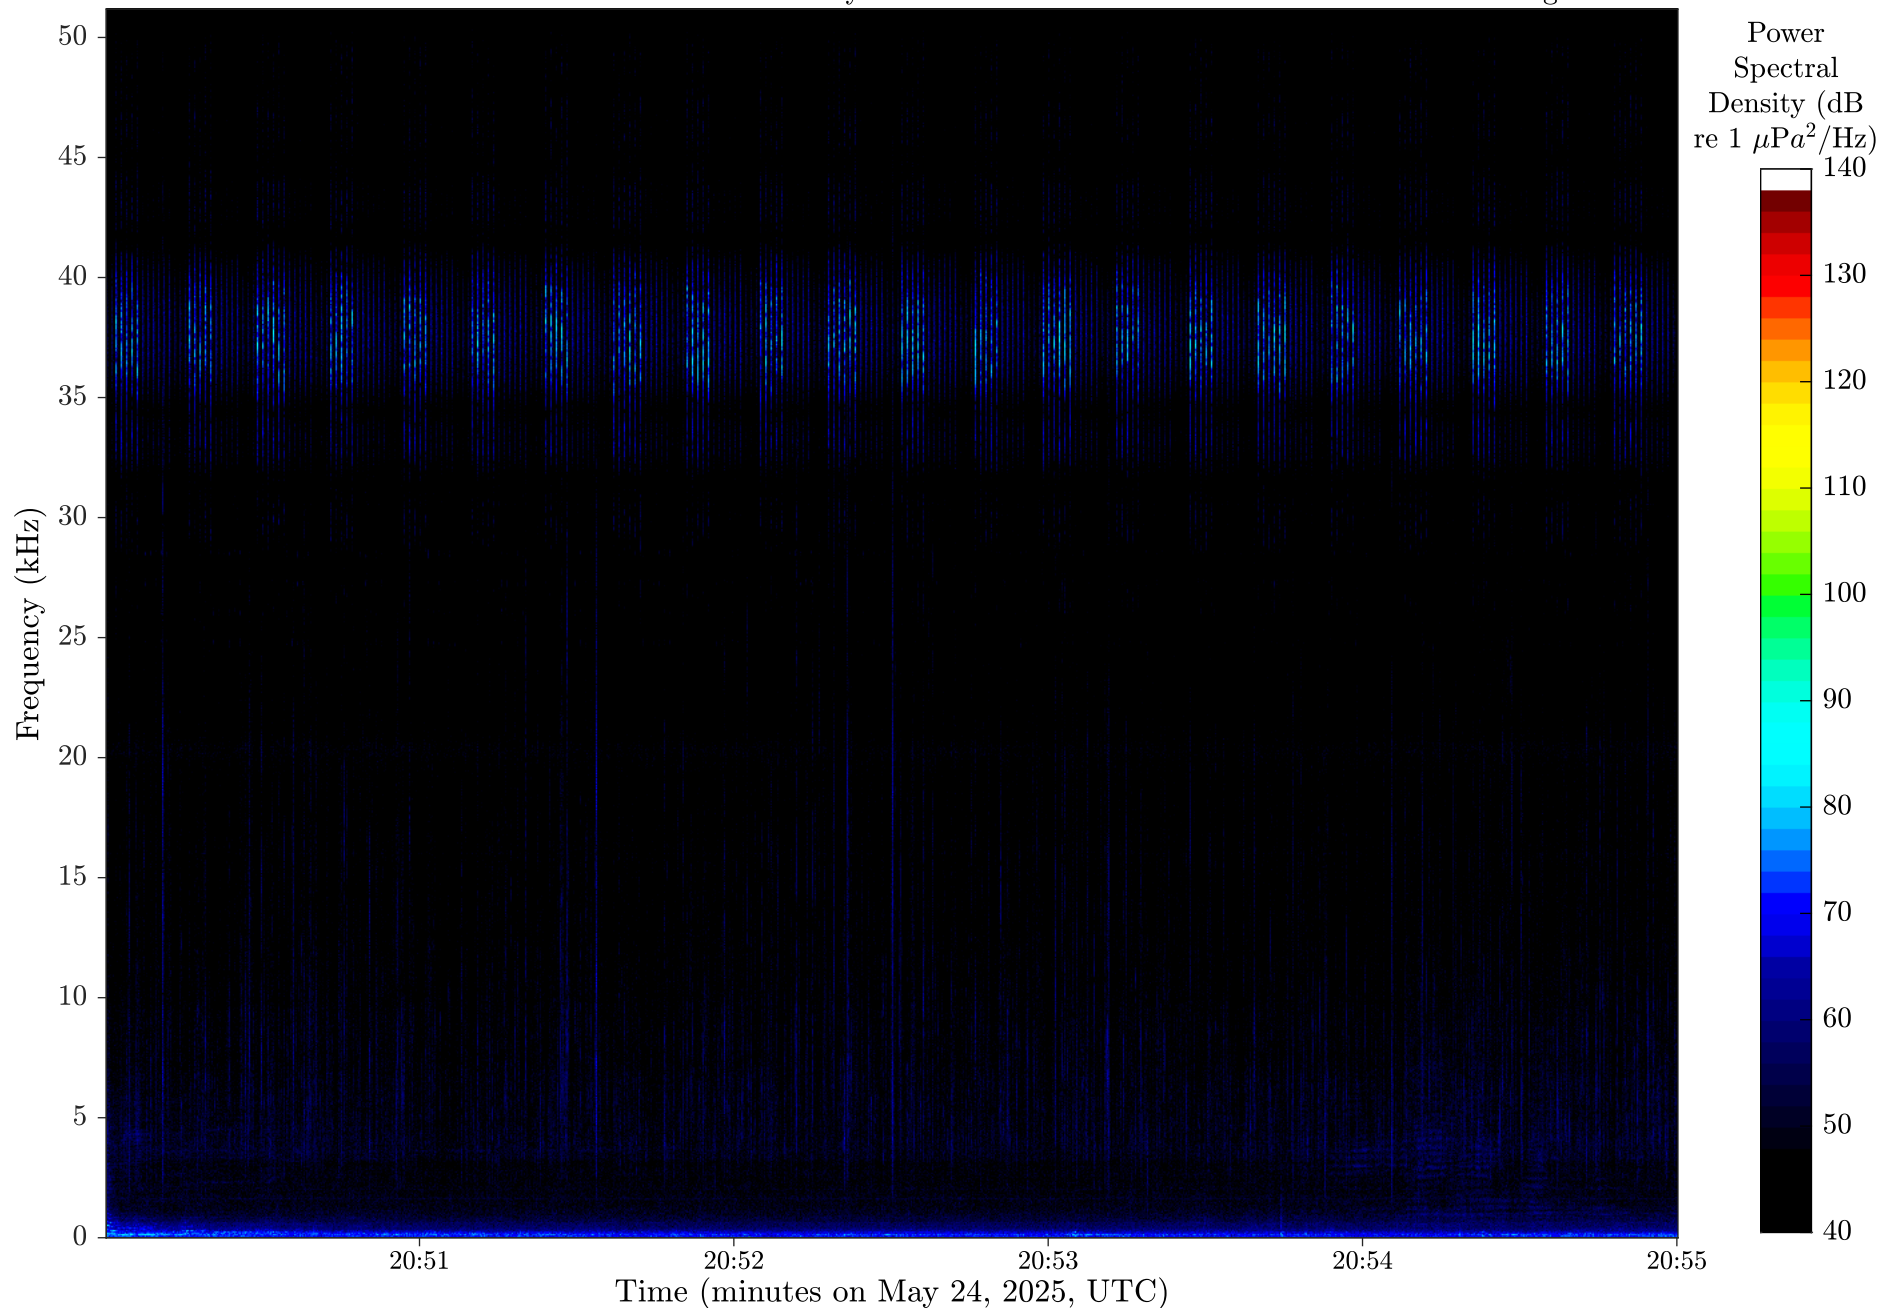

Comments: 33.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:41:22 UTC

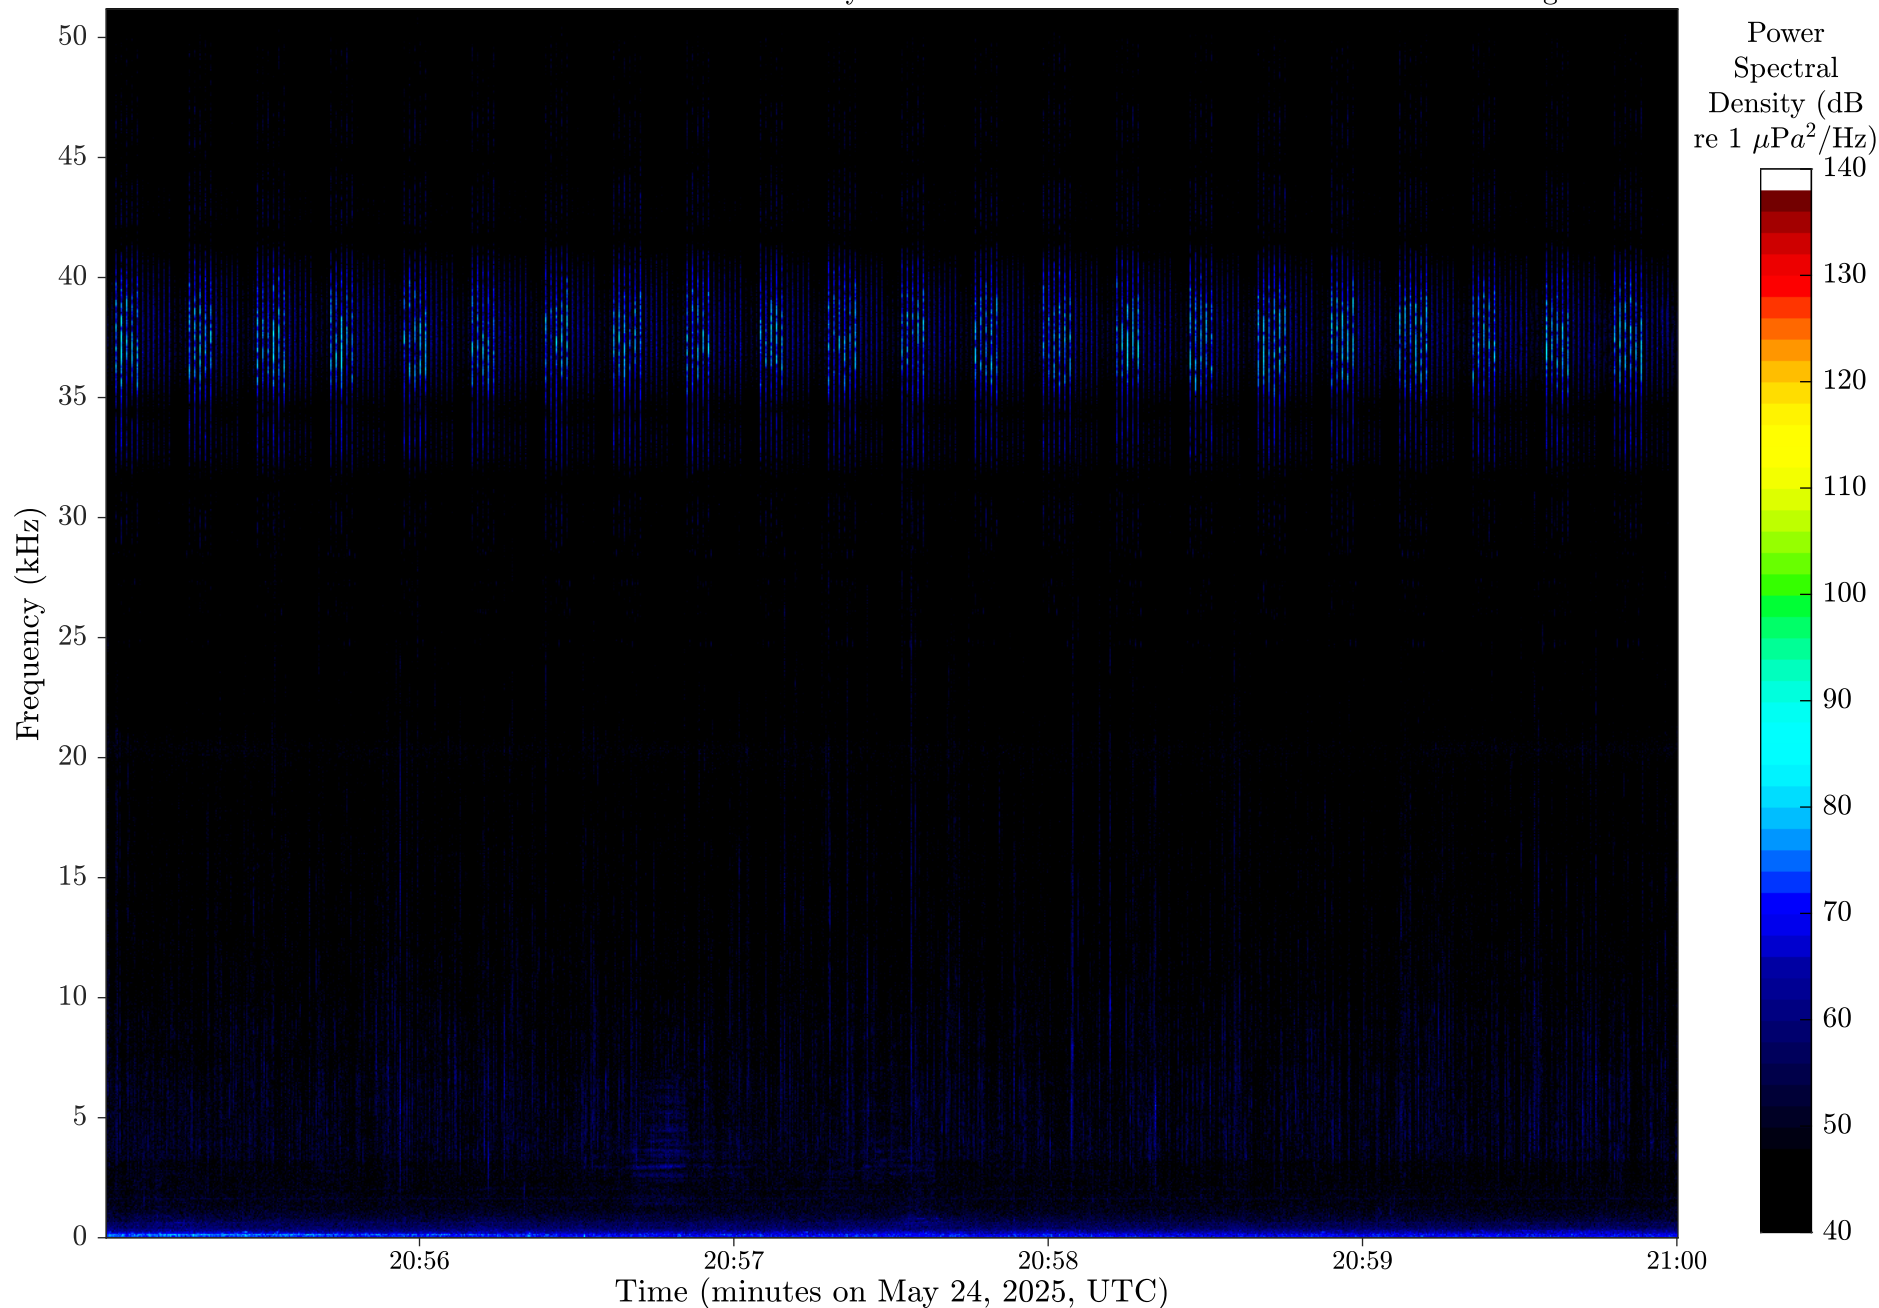

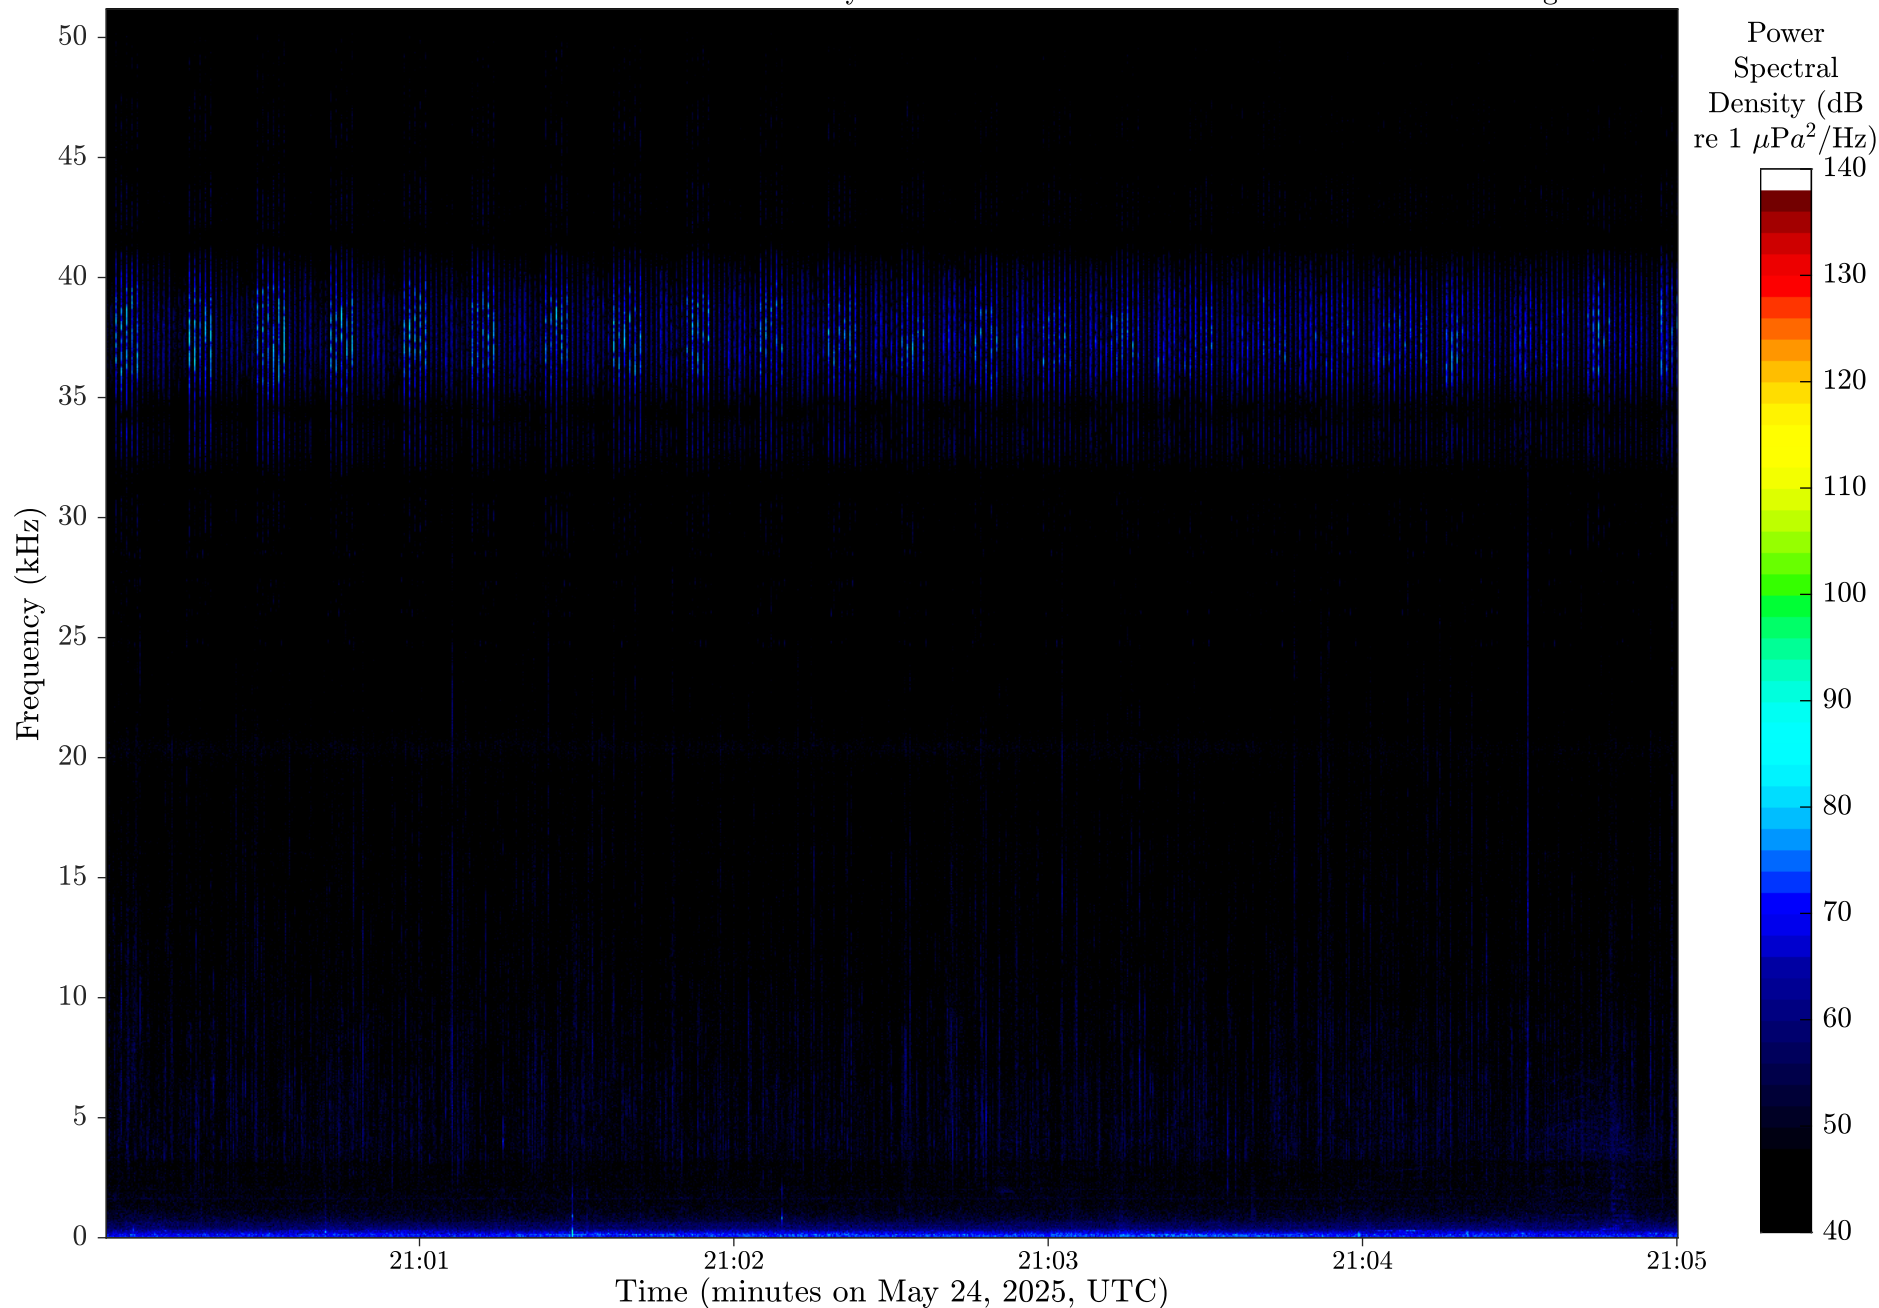


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:40 UTC

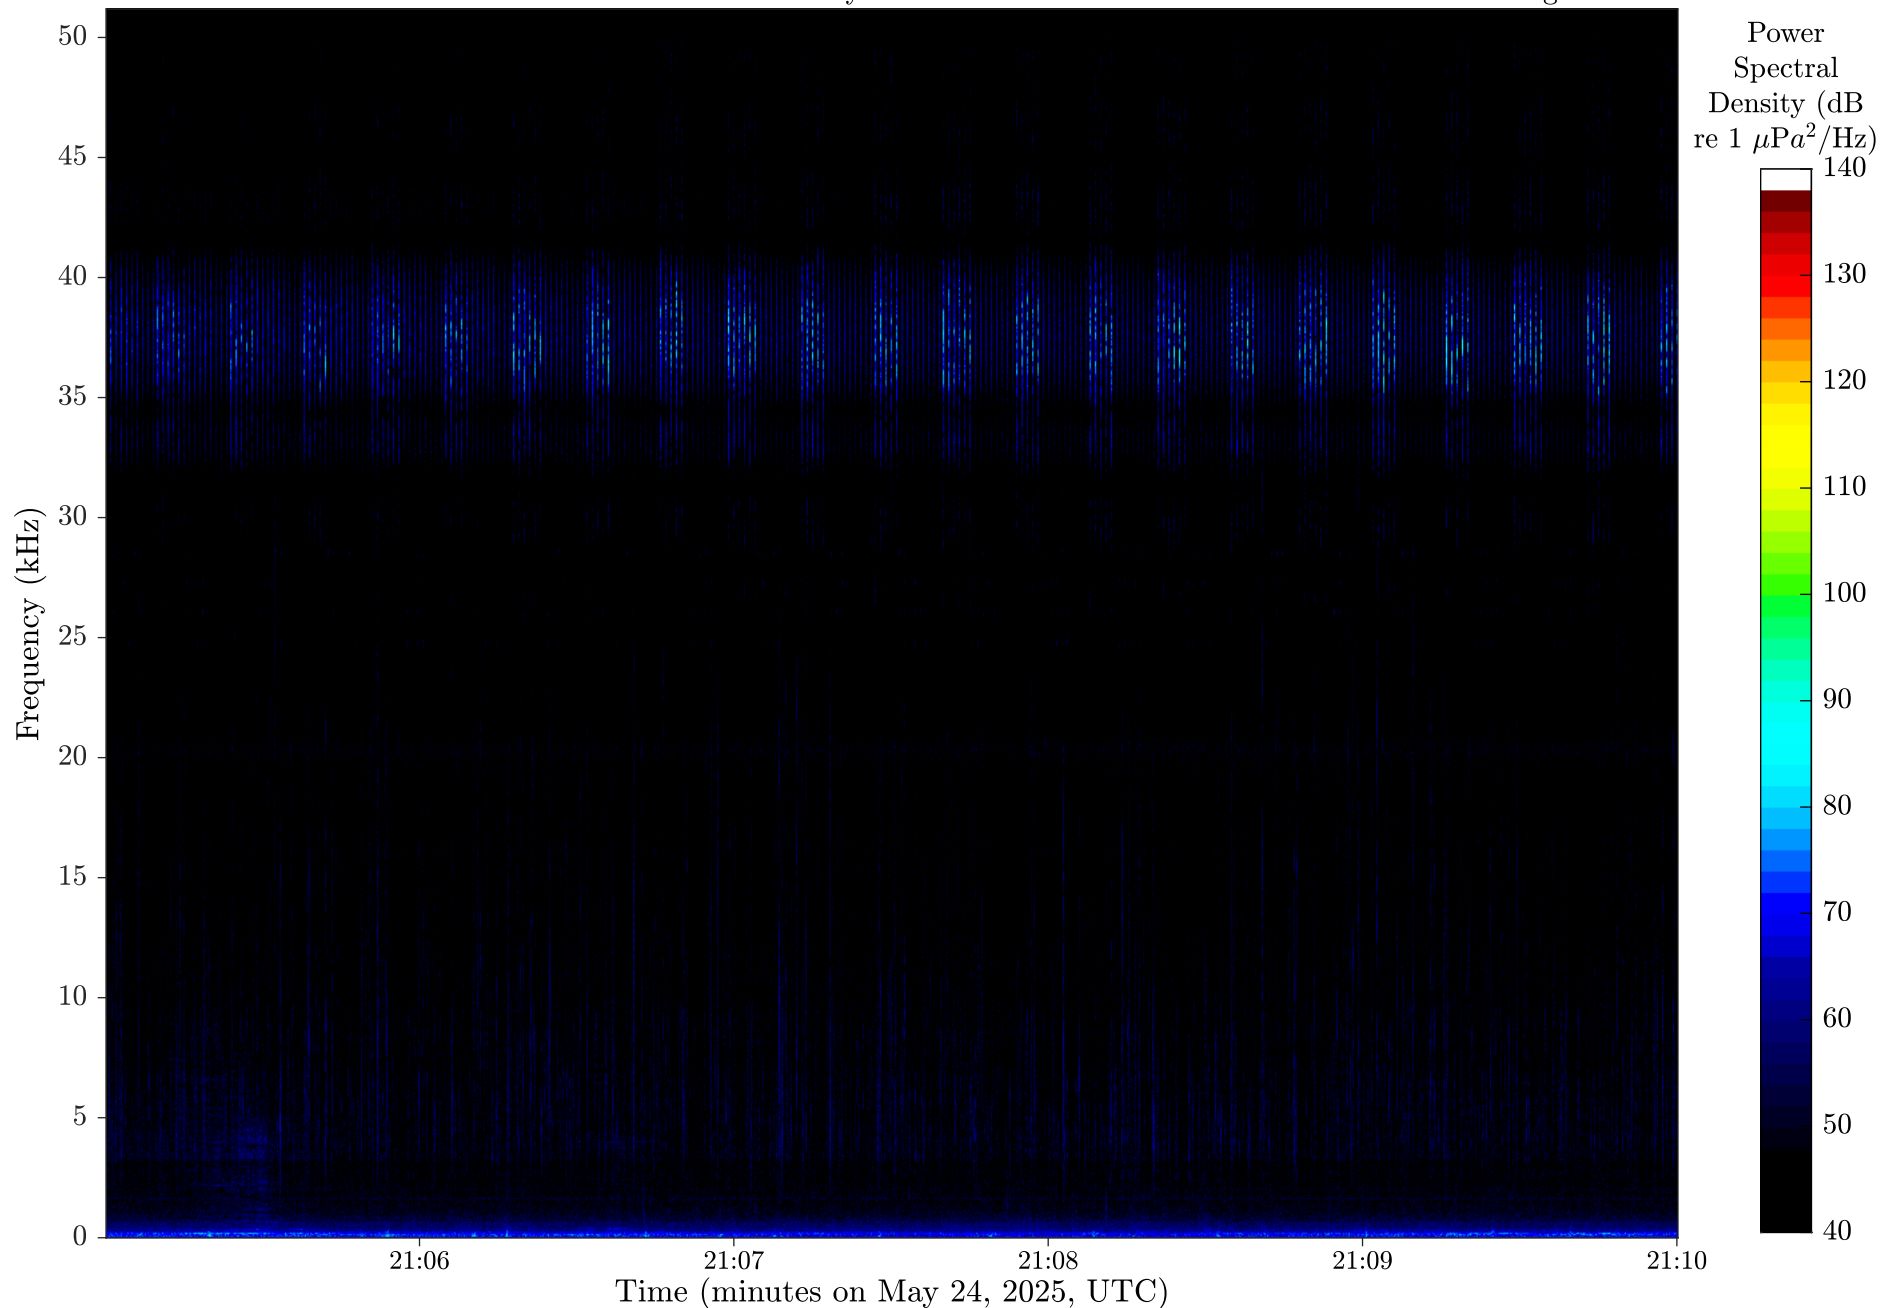


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:48 UTC

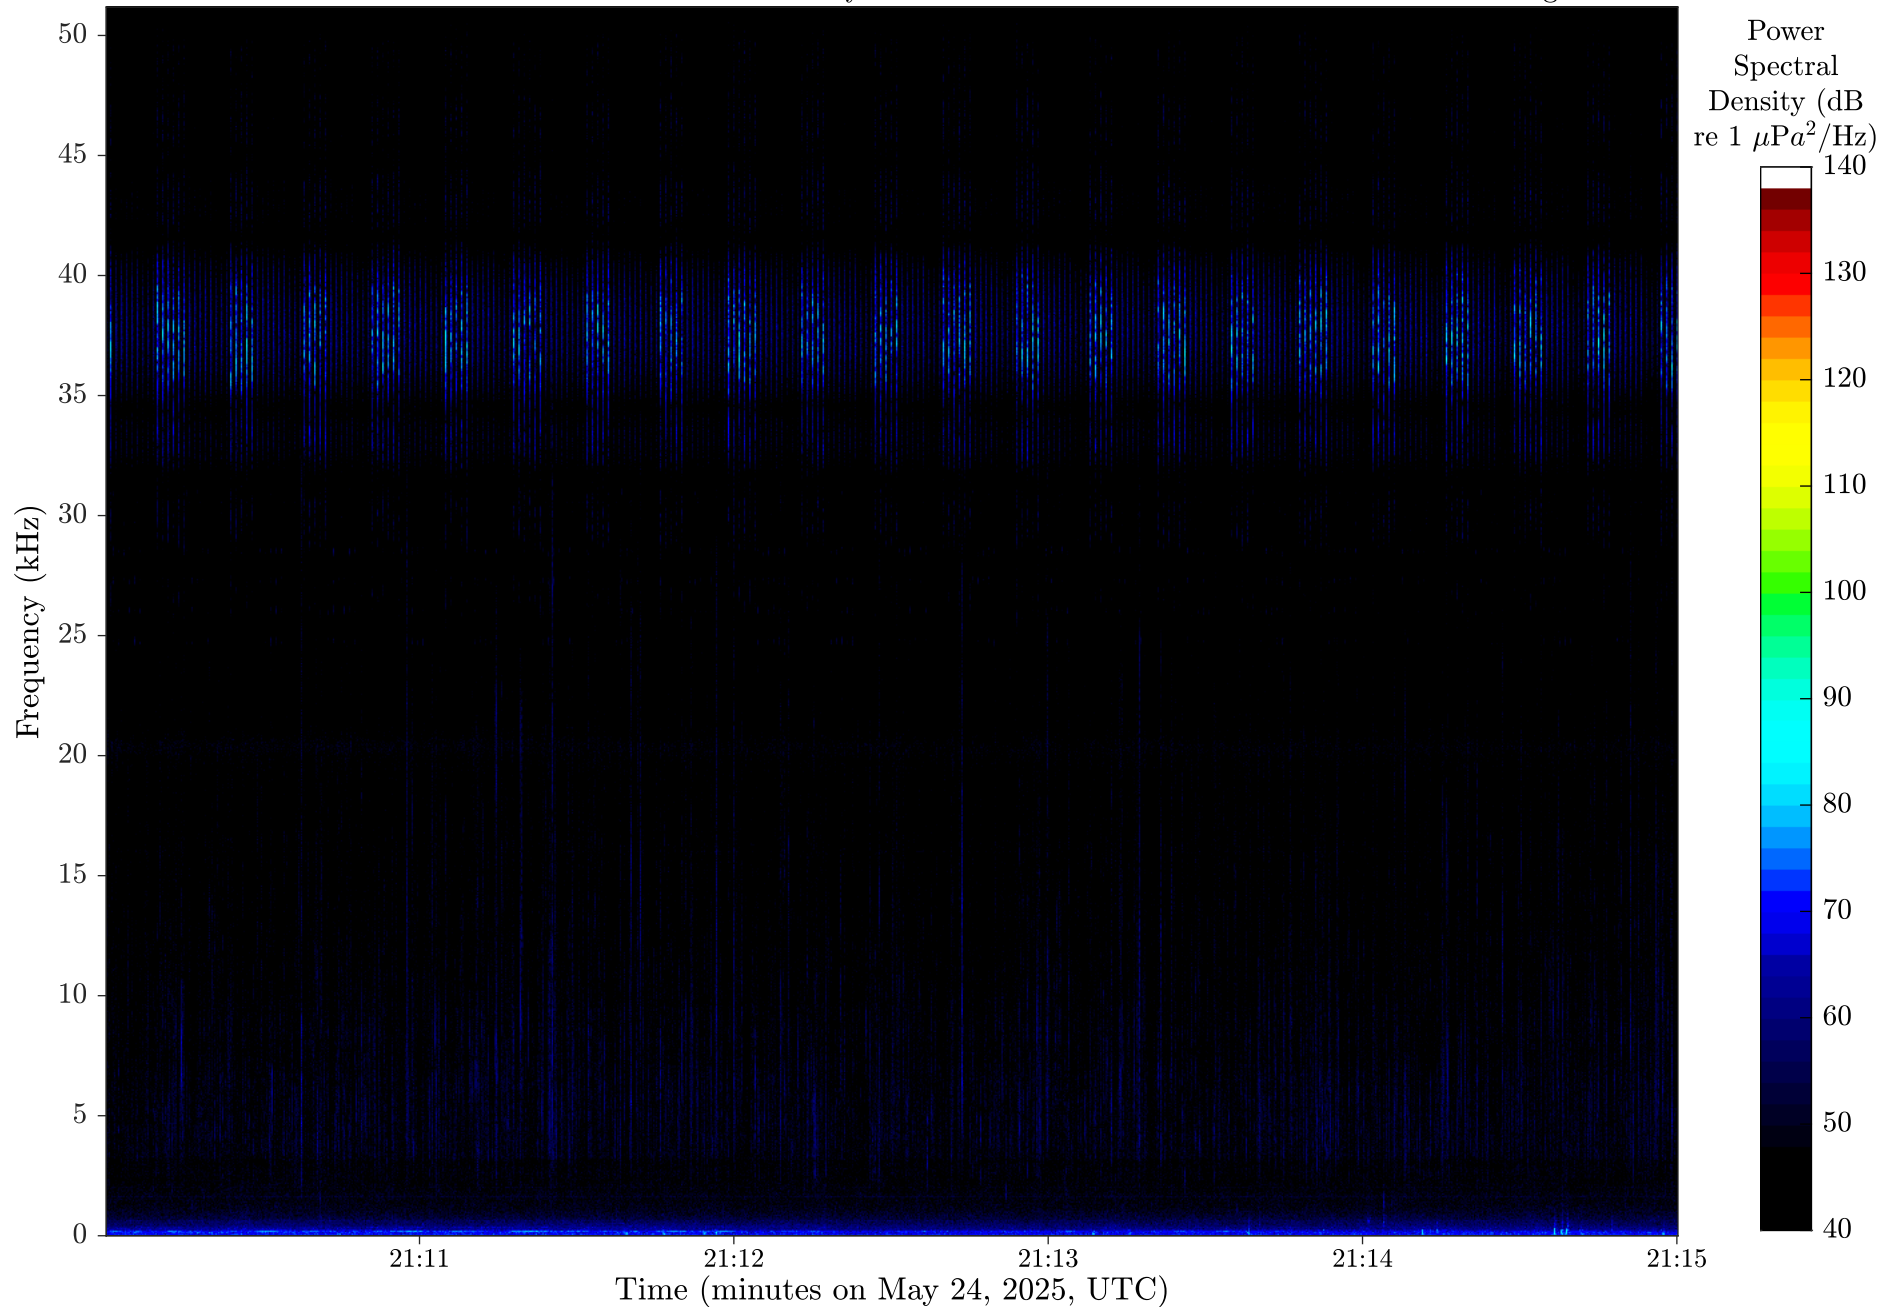


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:41:56 UTC

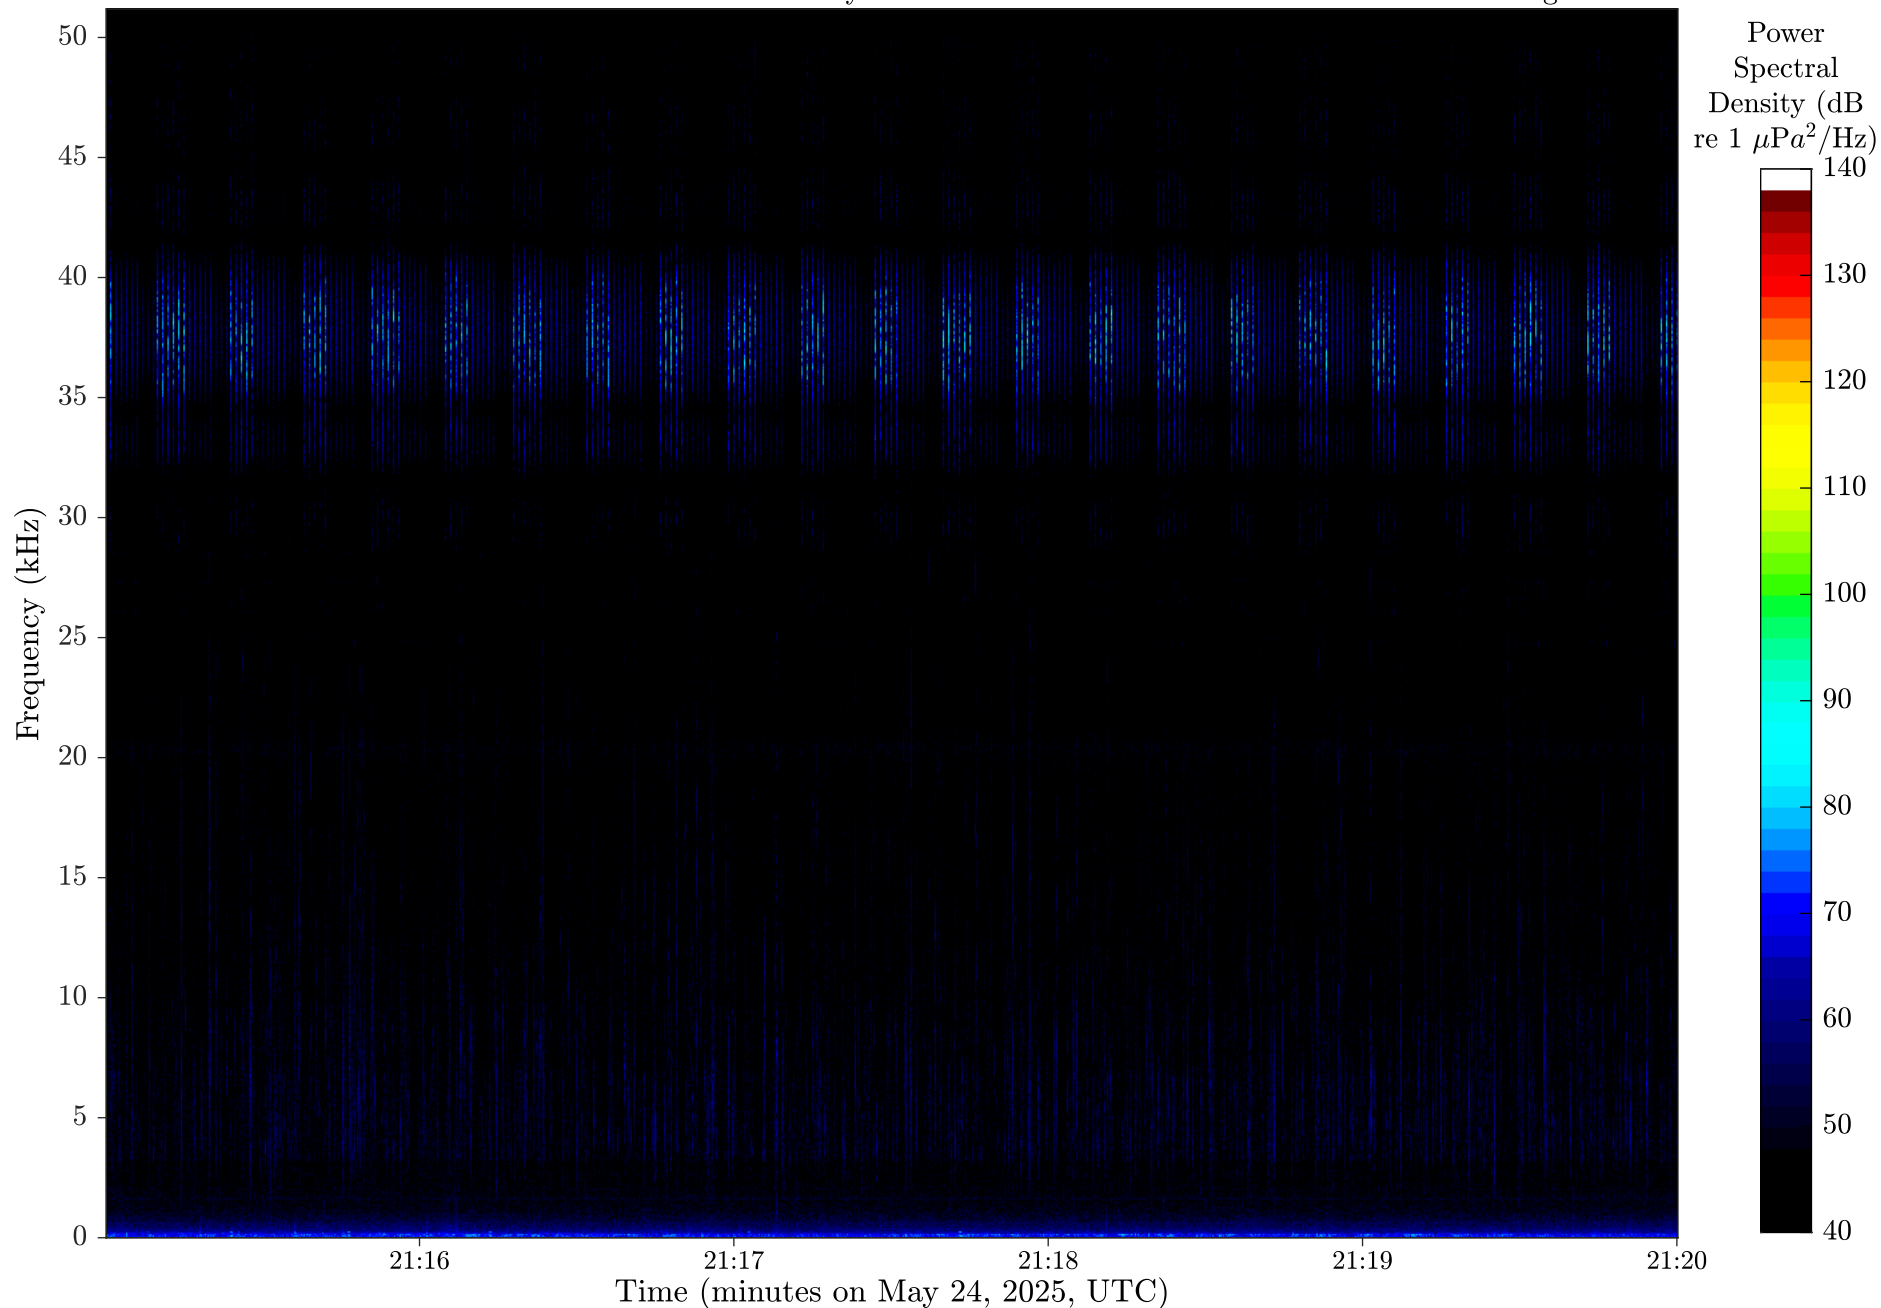


Comments: 34.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:03 UTC

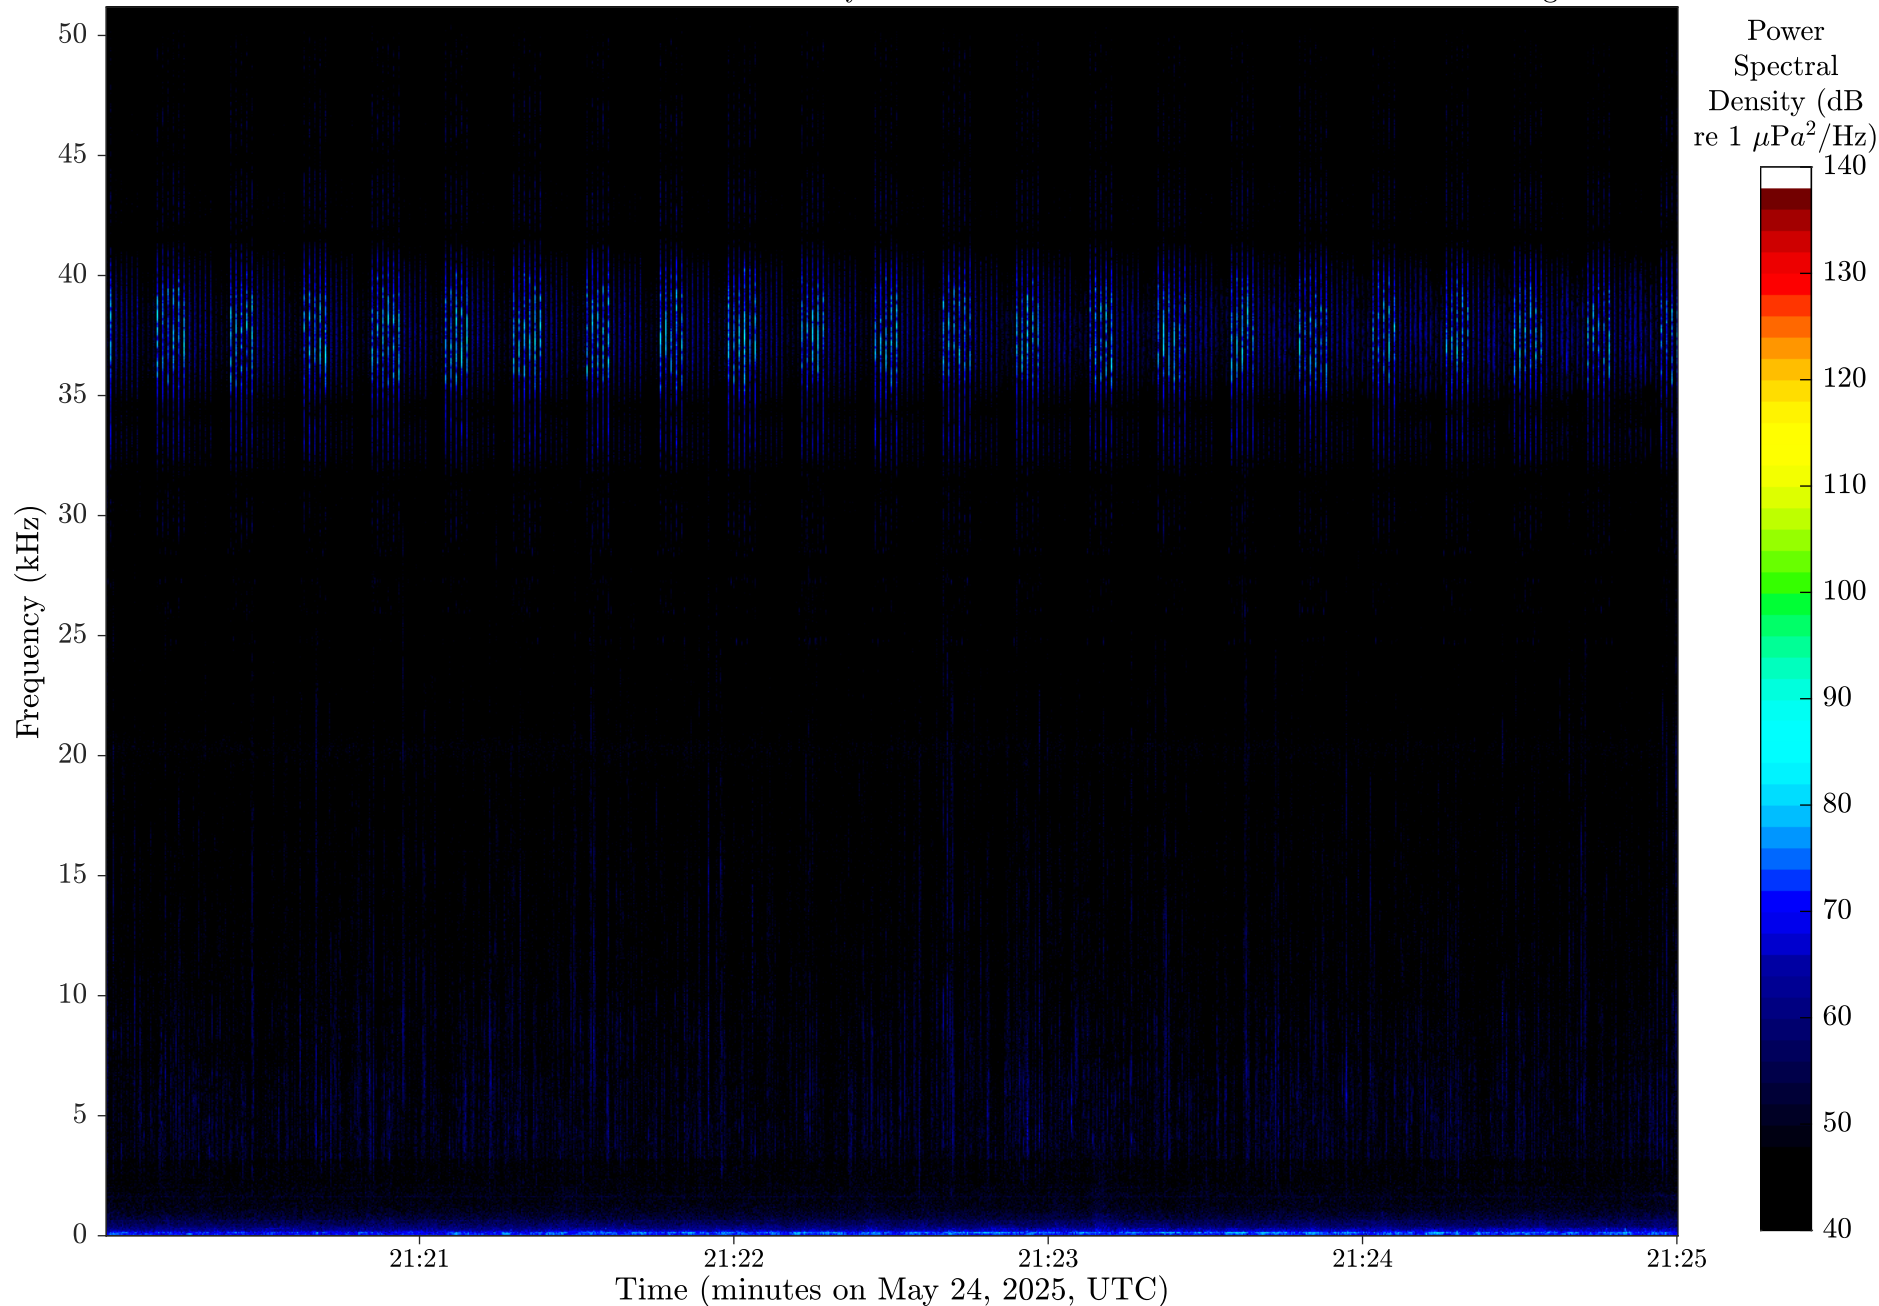


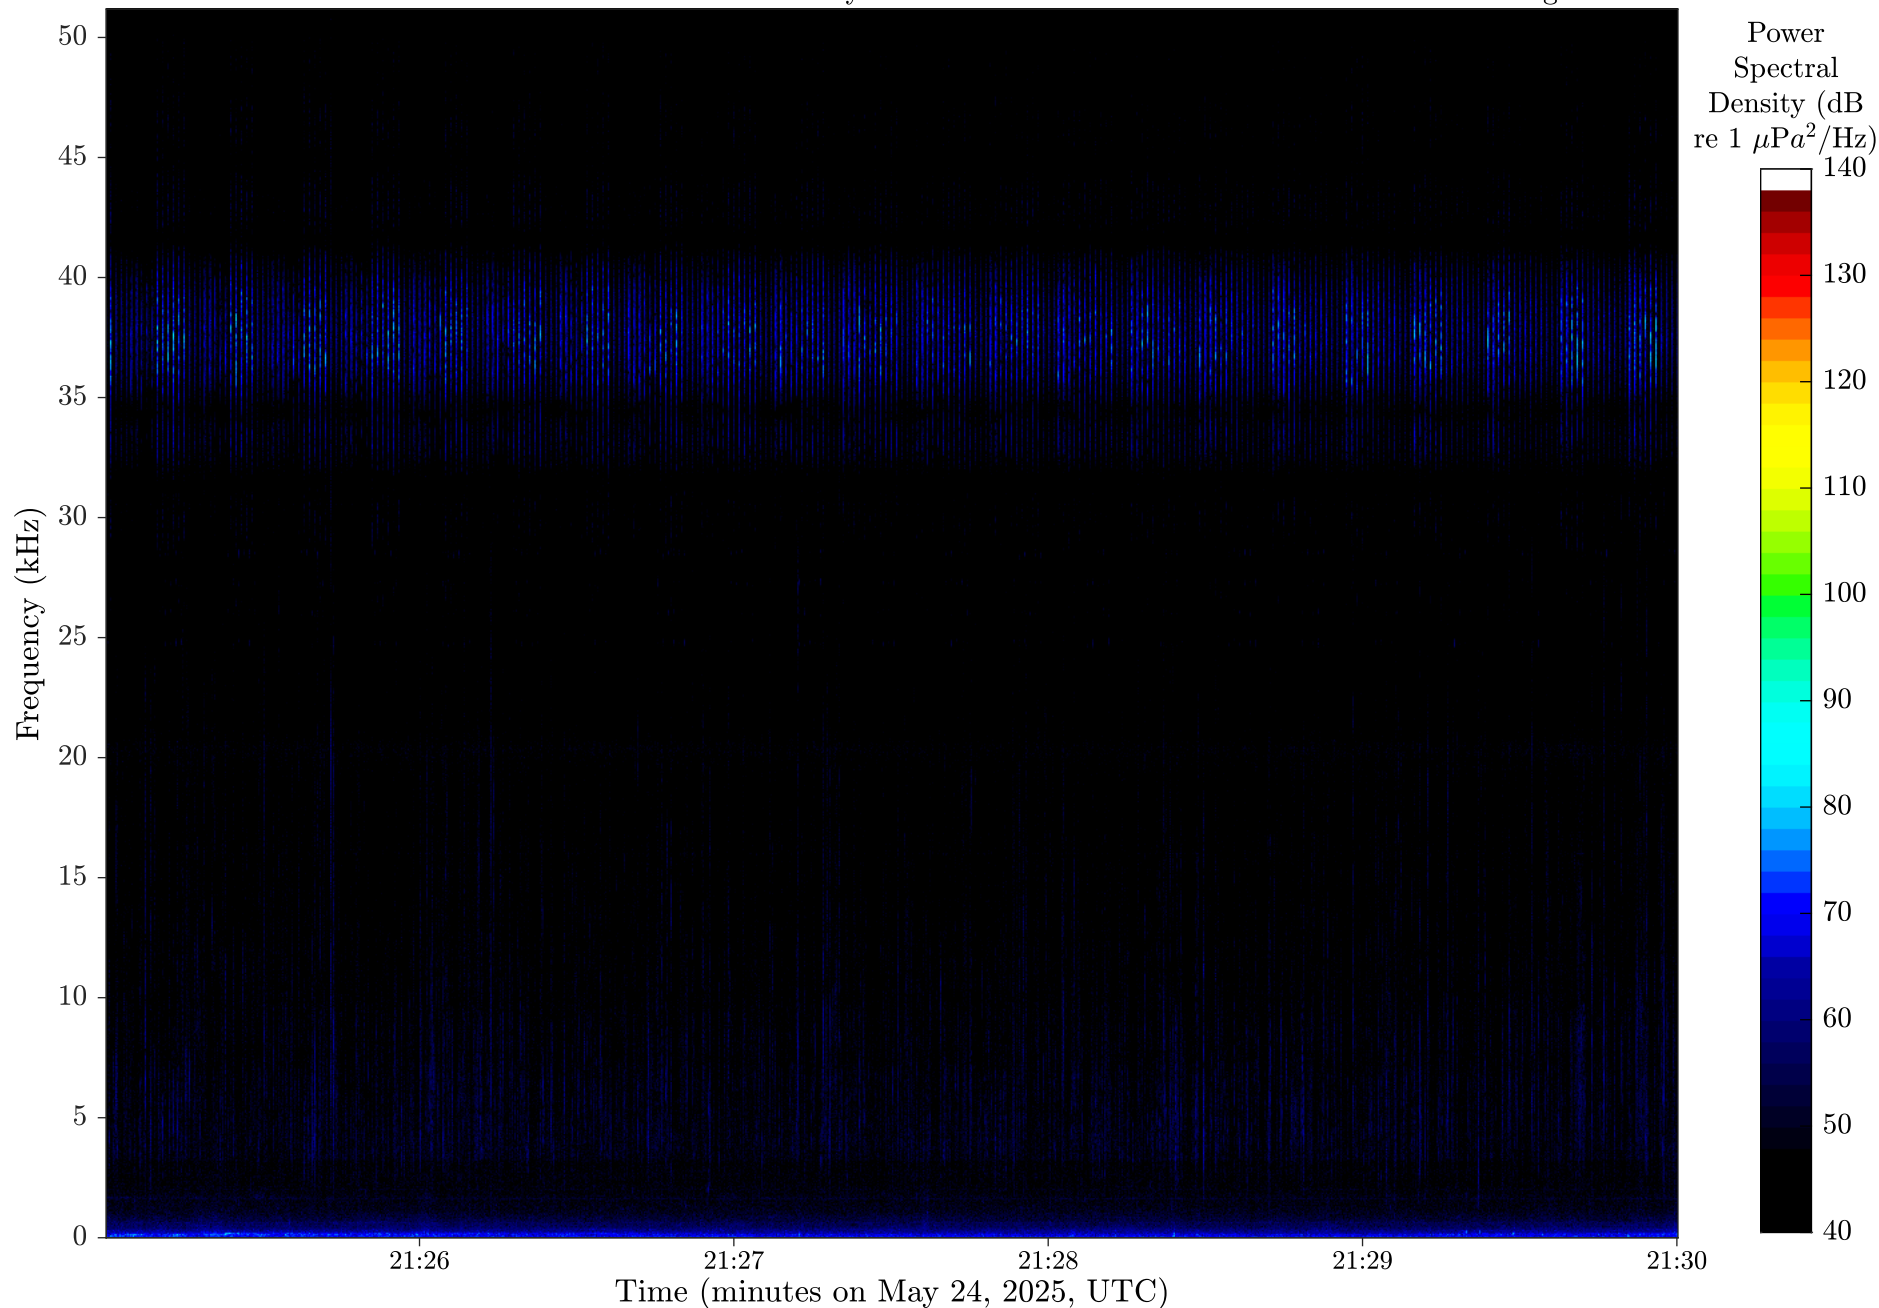

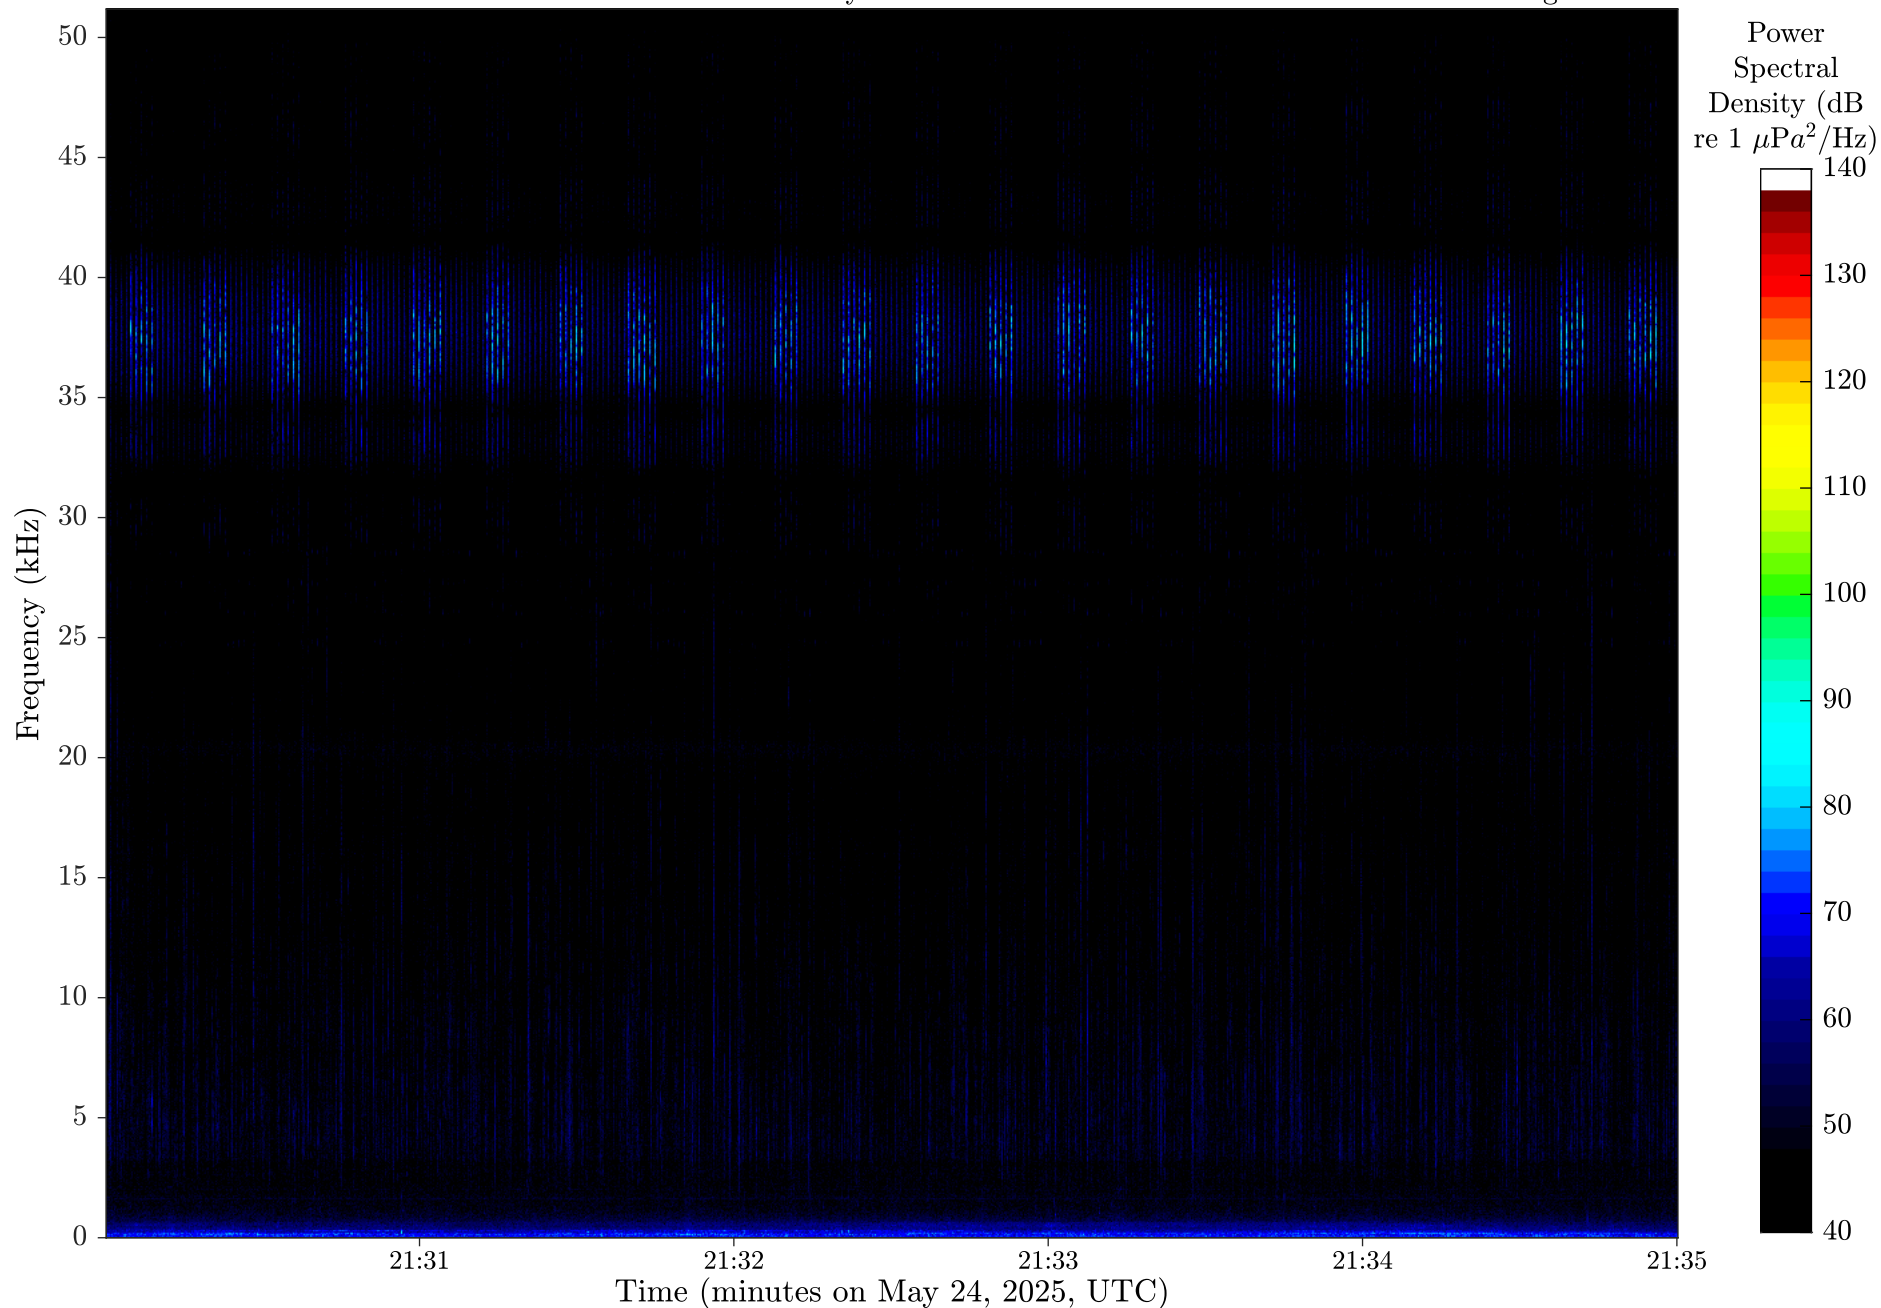


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:26 UTC

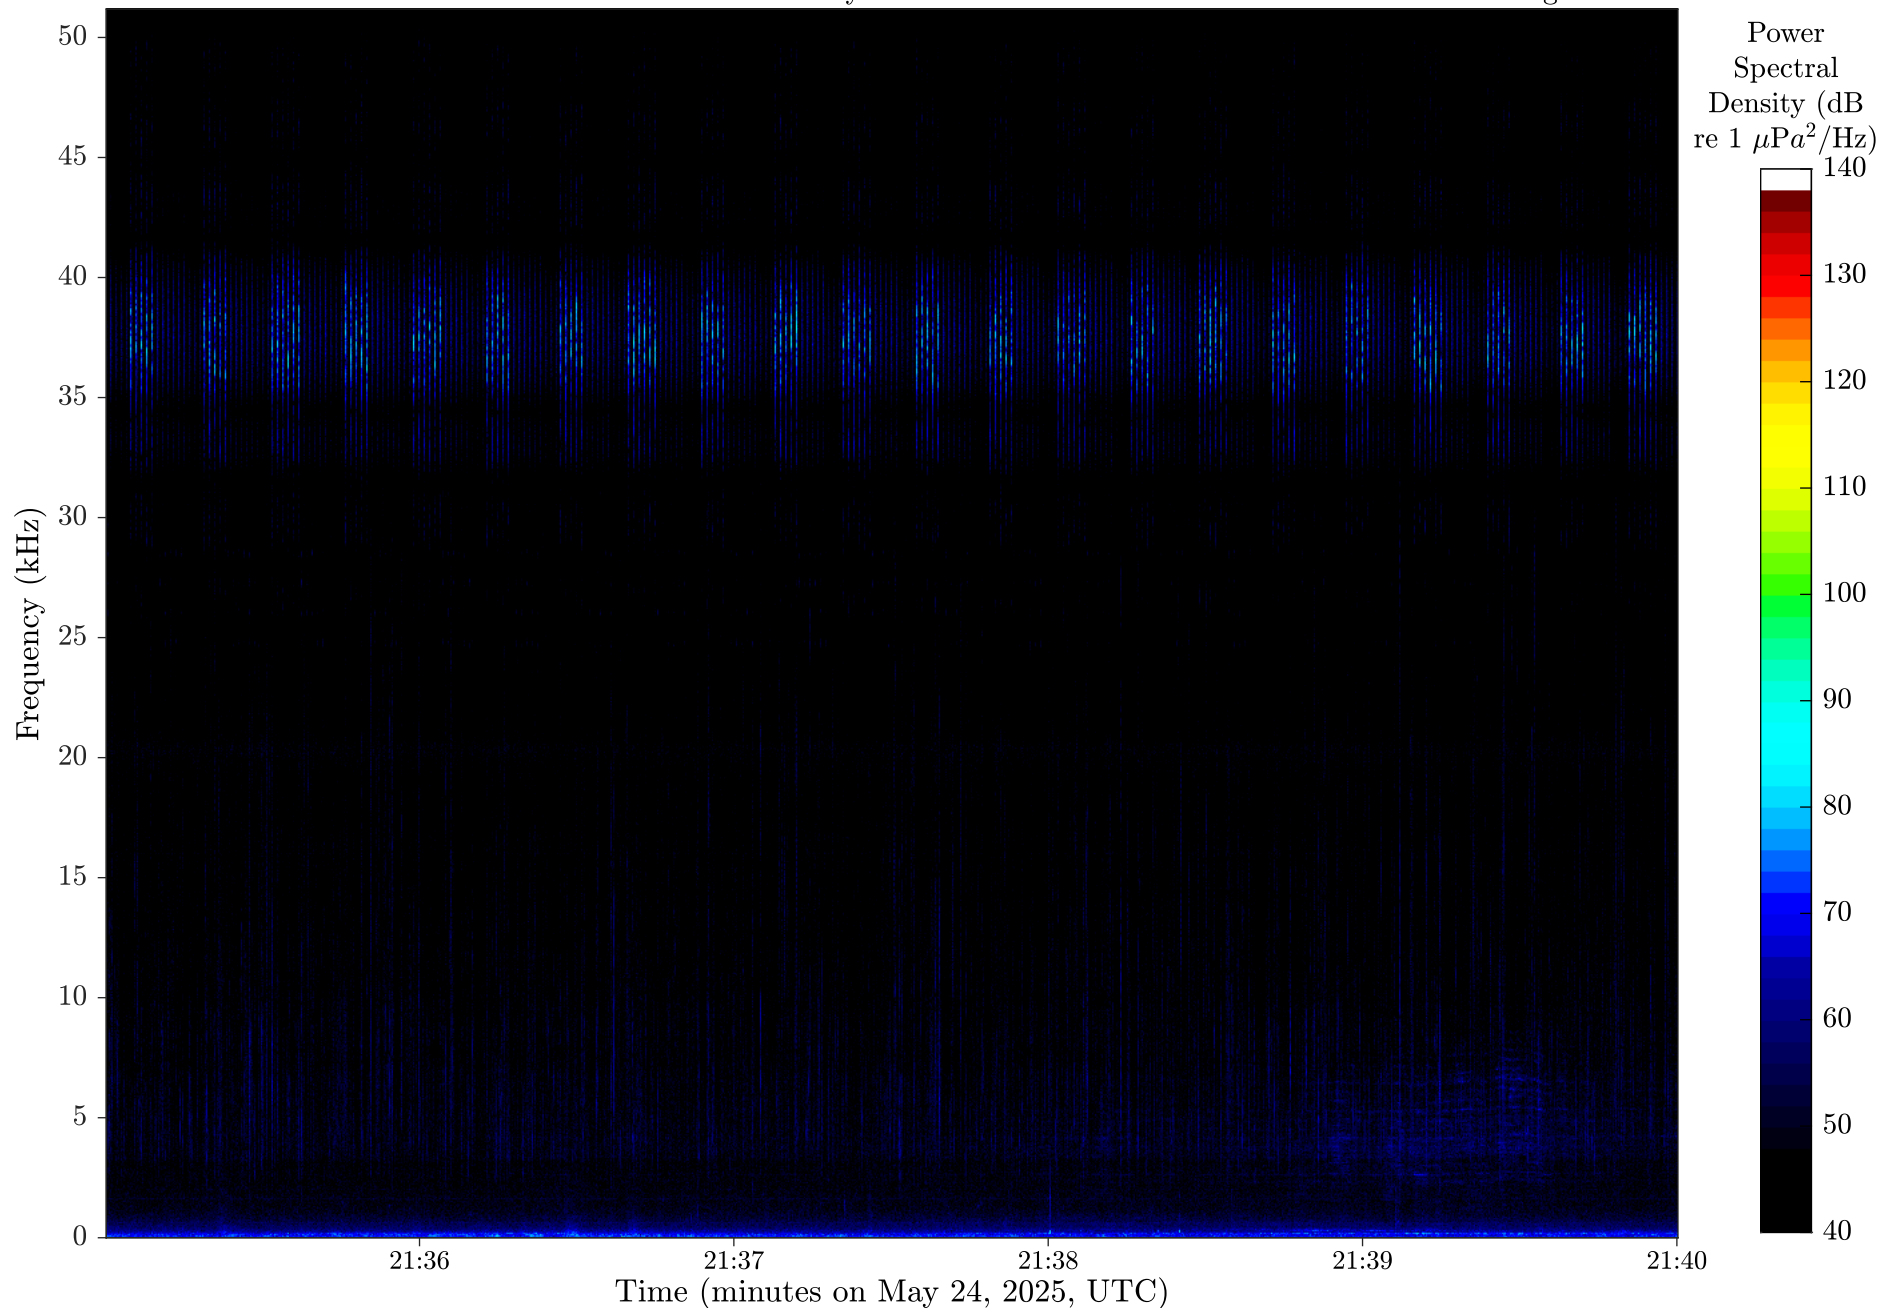


Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:34 UTC

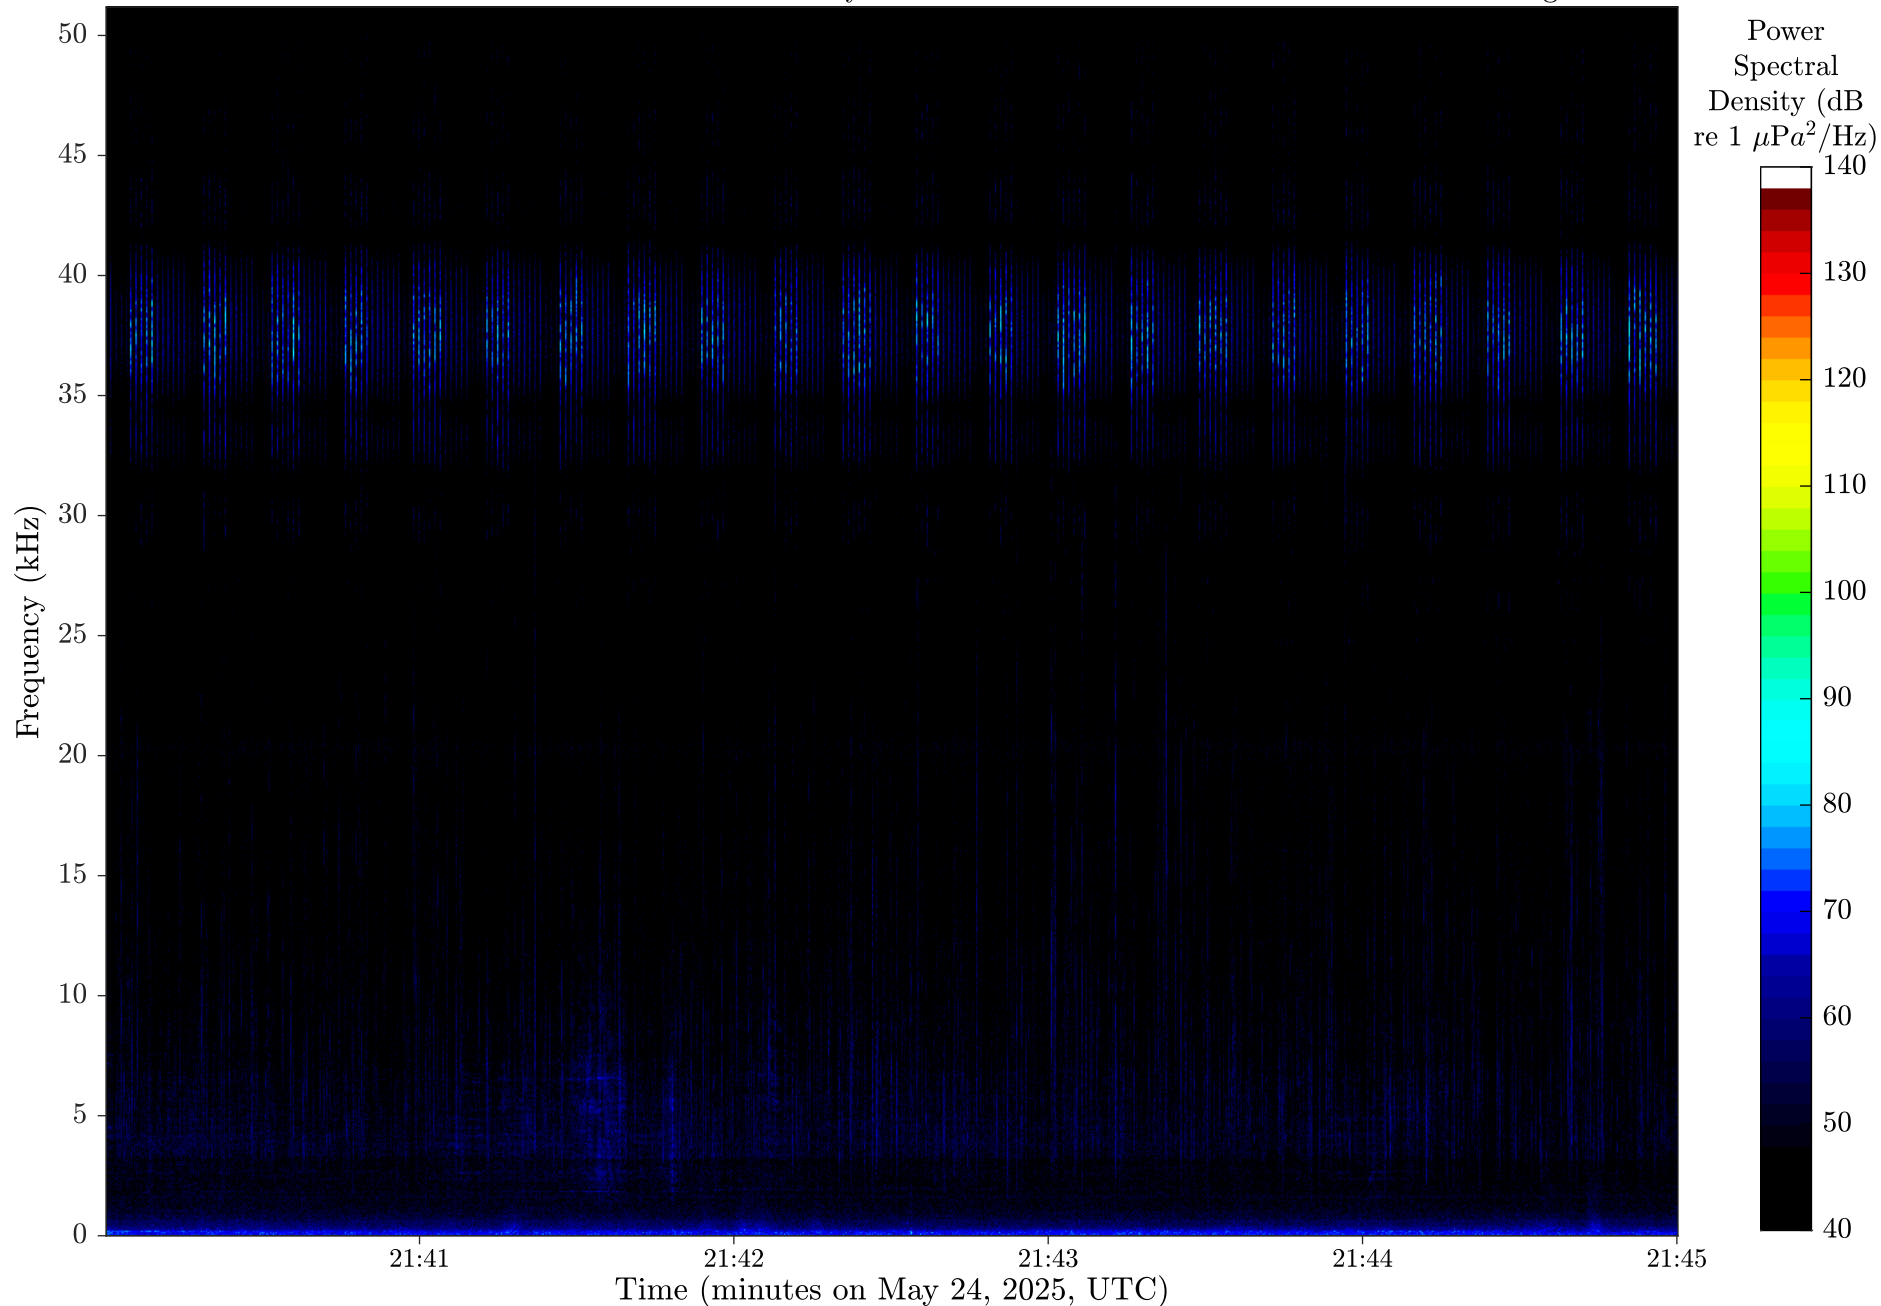


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:41 UTC

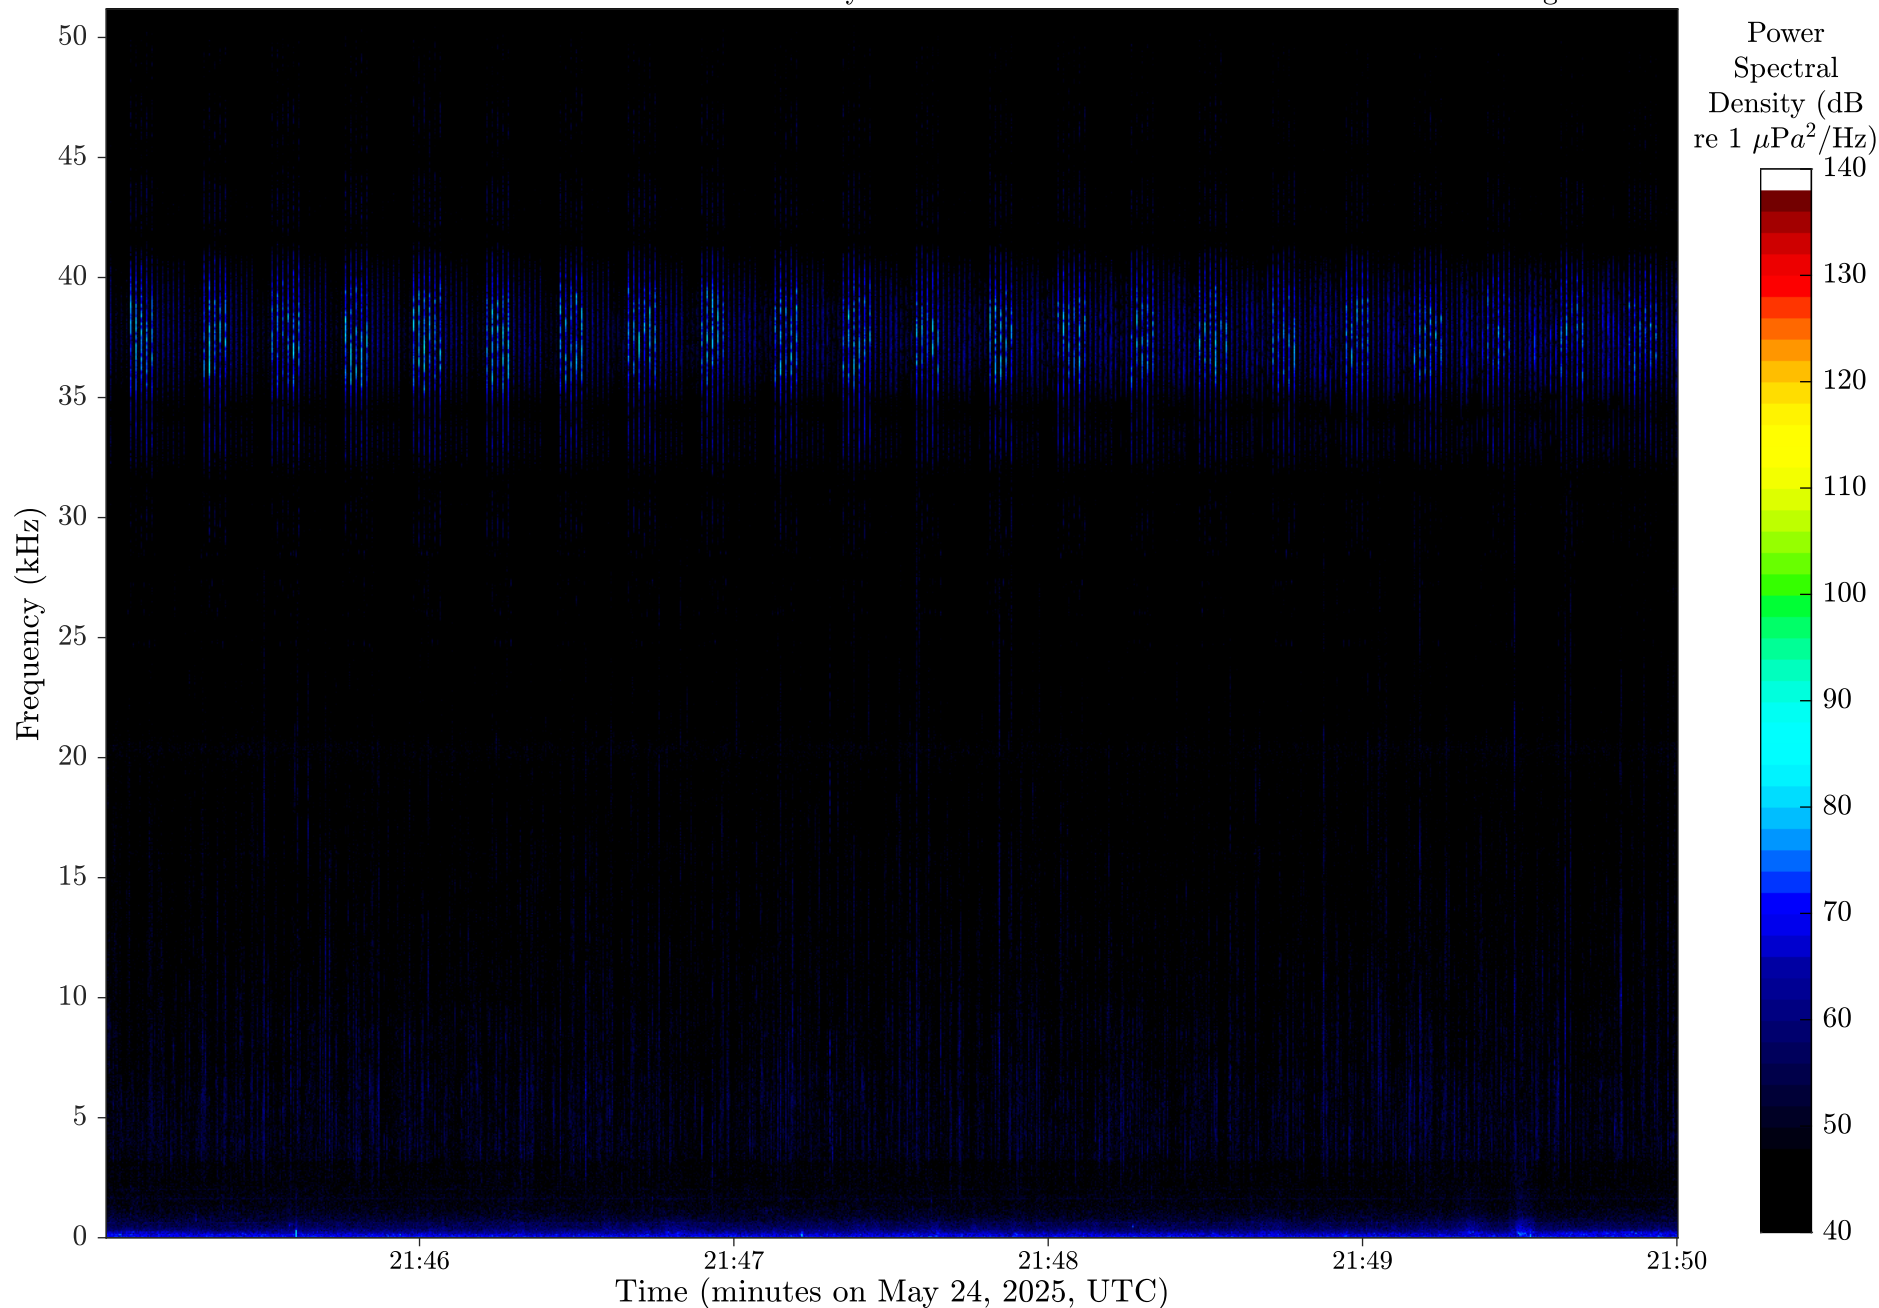


Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:42:50 UTC

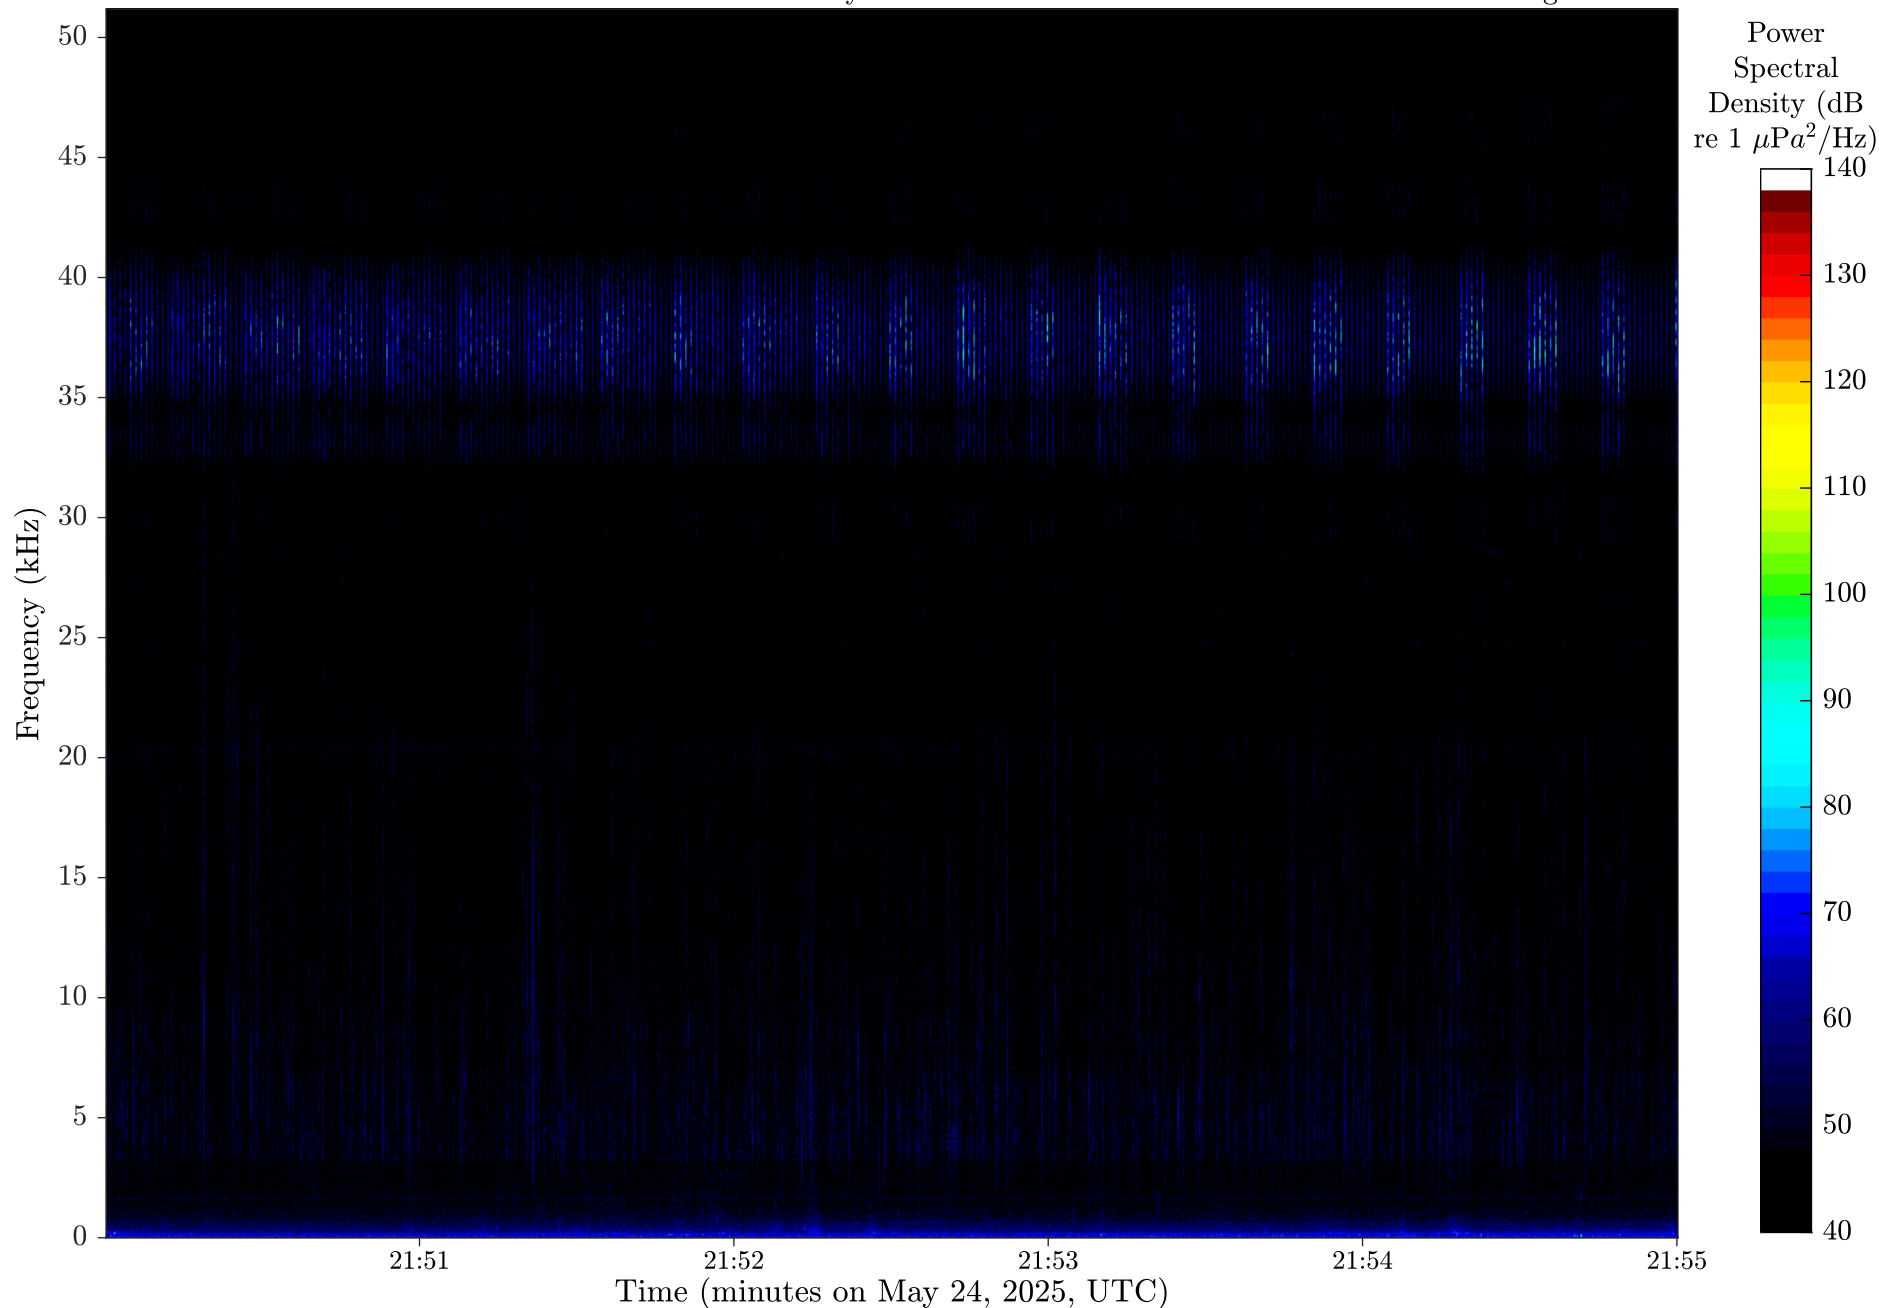

Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:42:57 UTC

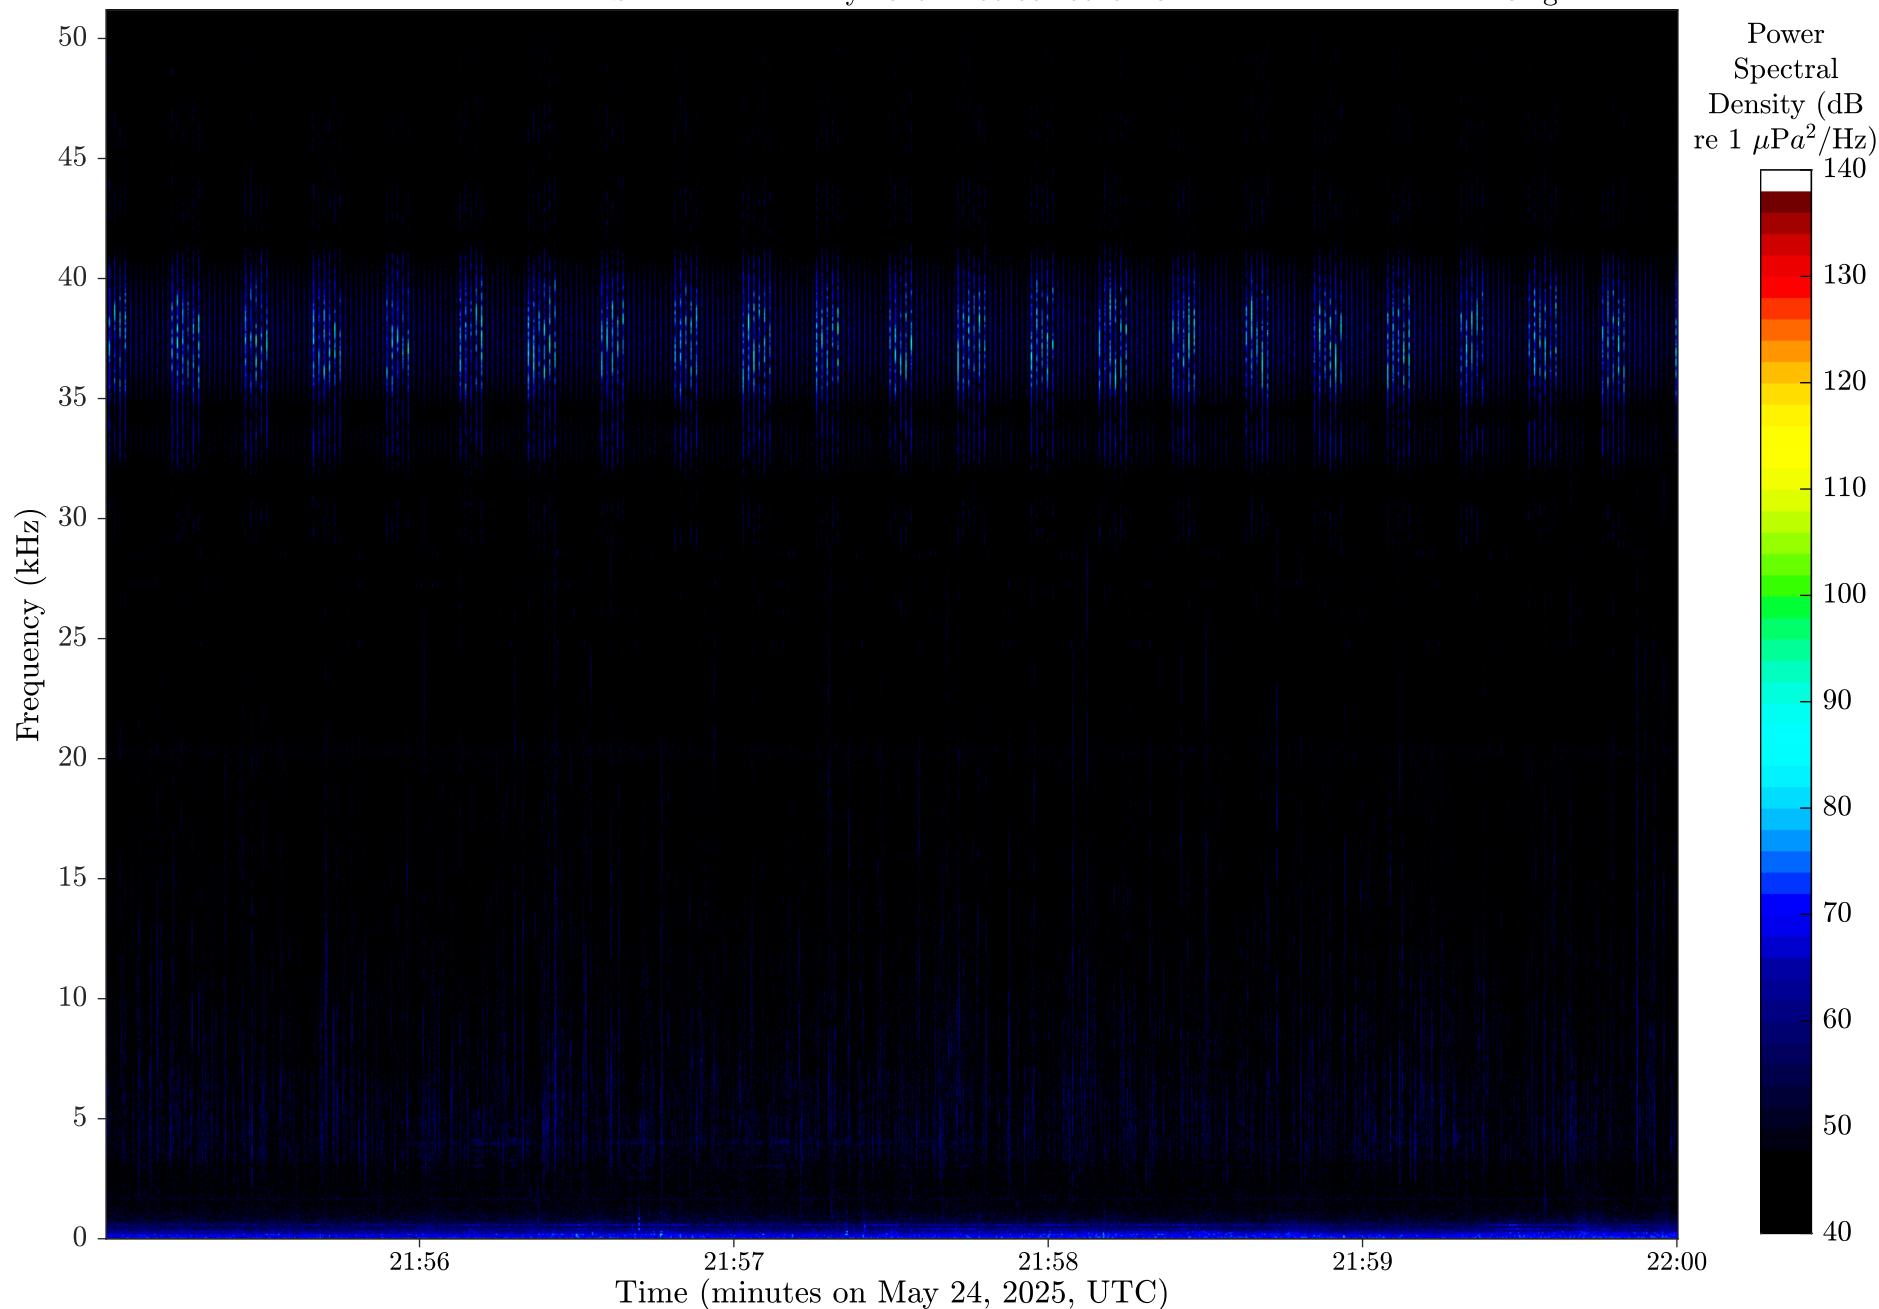

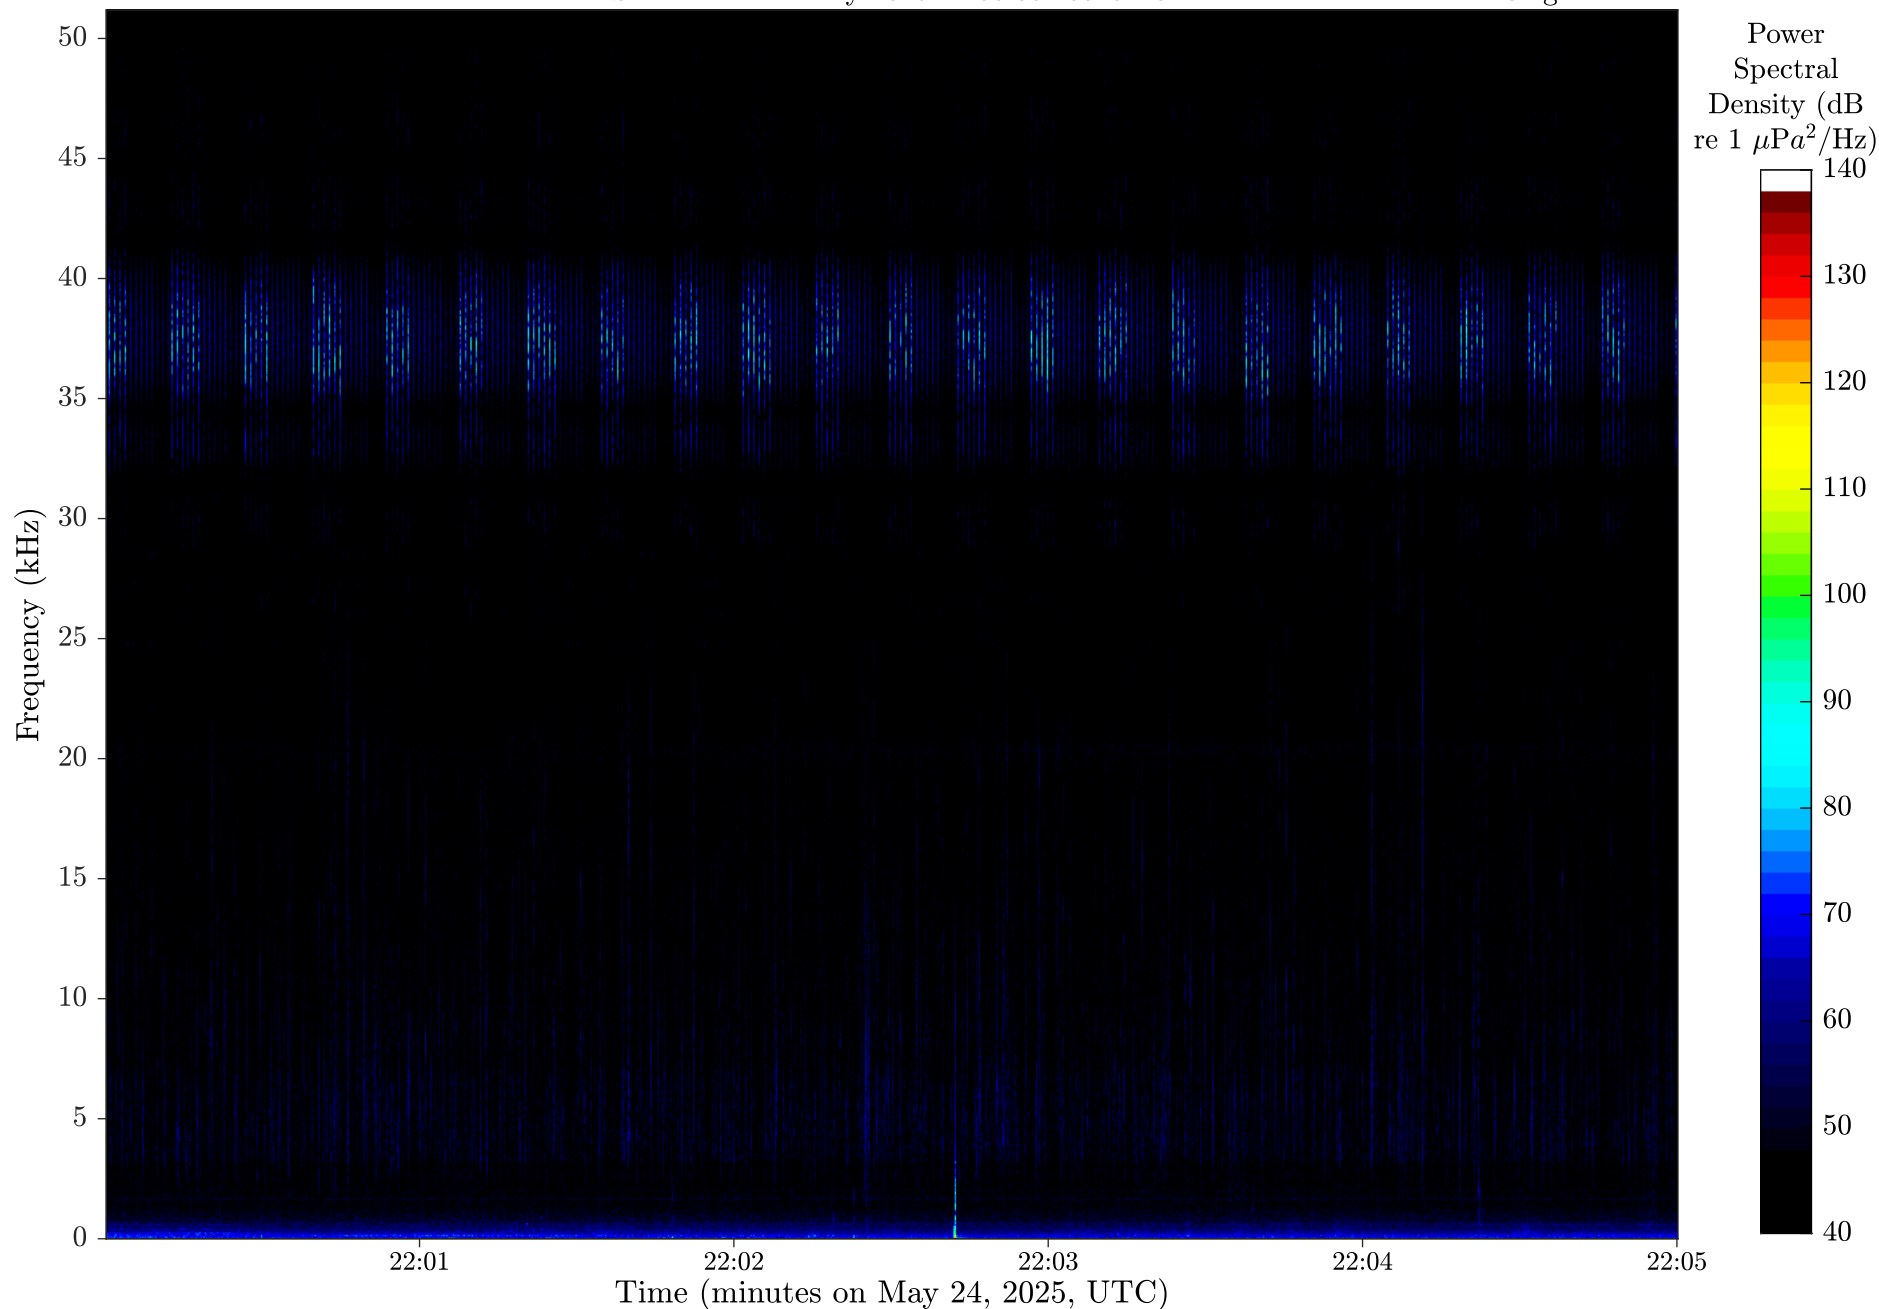


Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:43:12 UTC

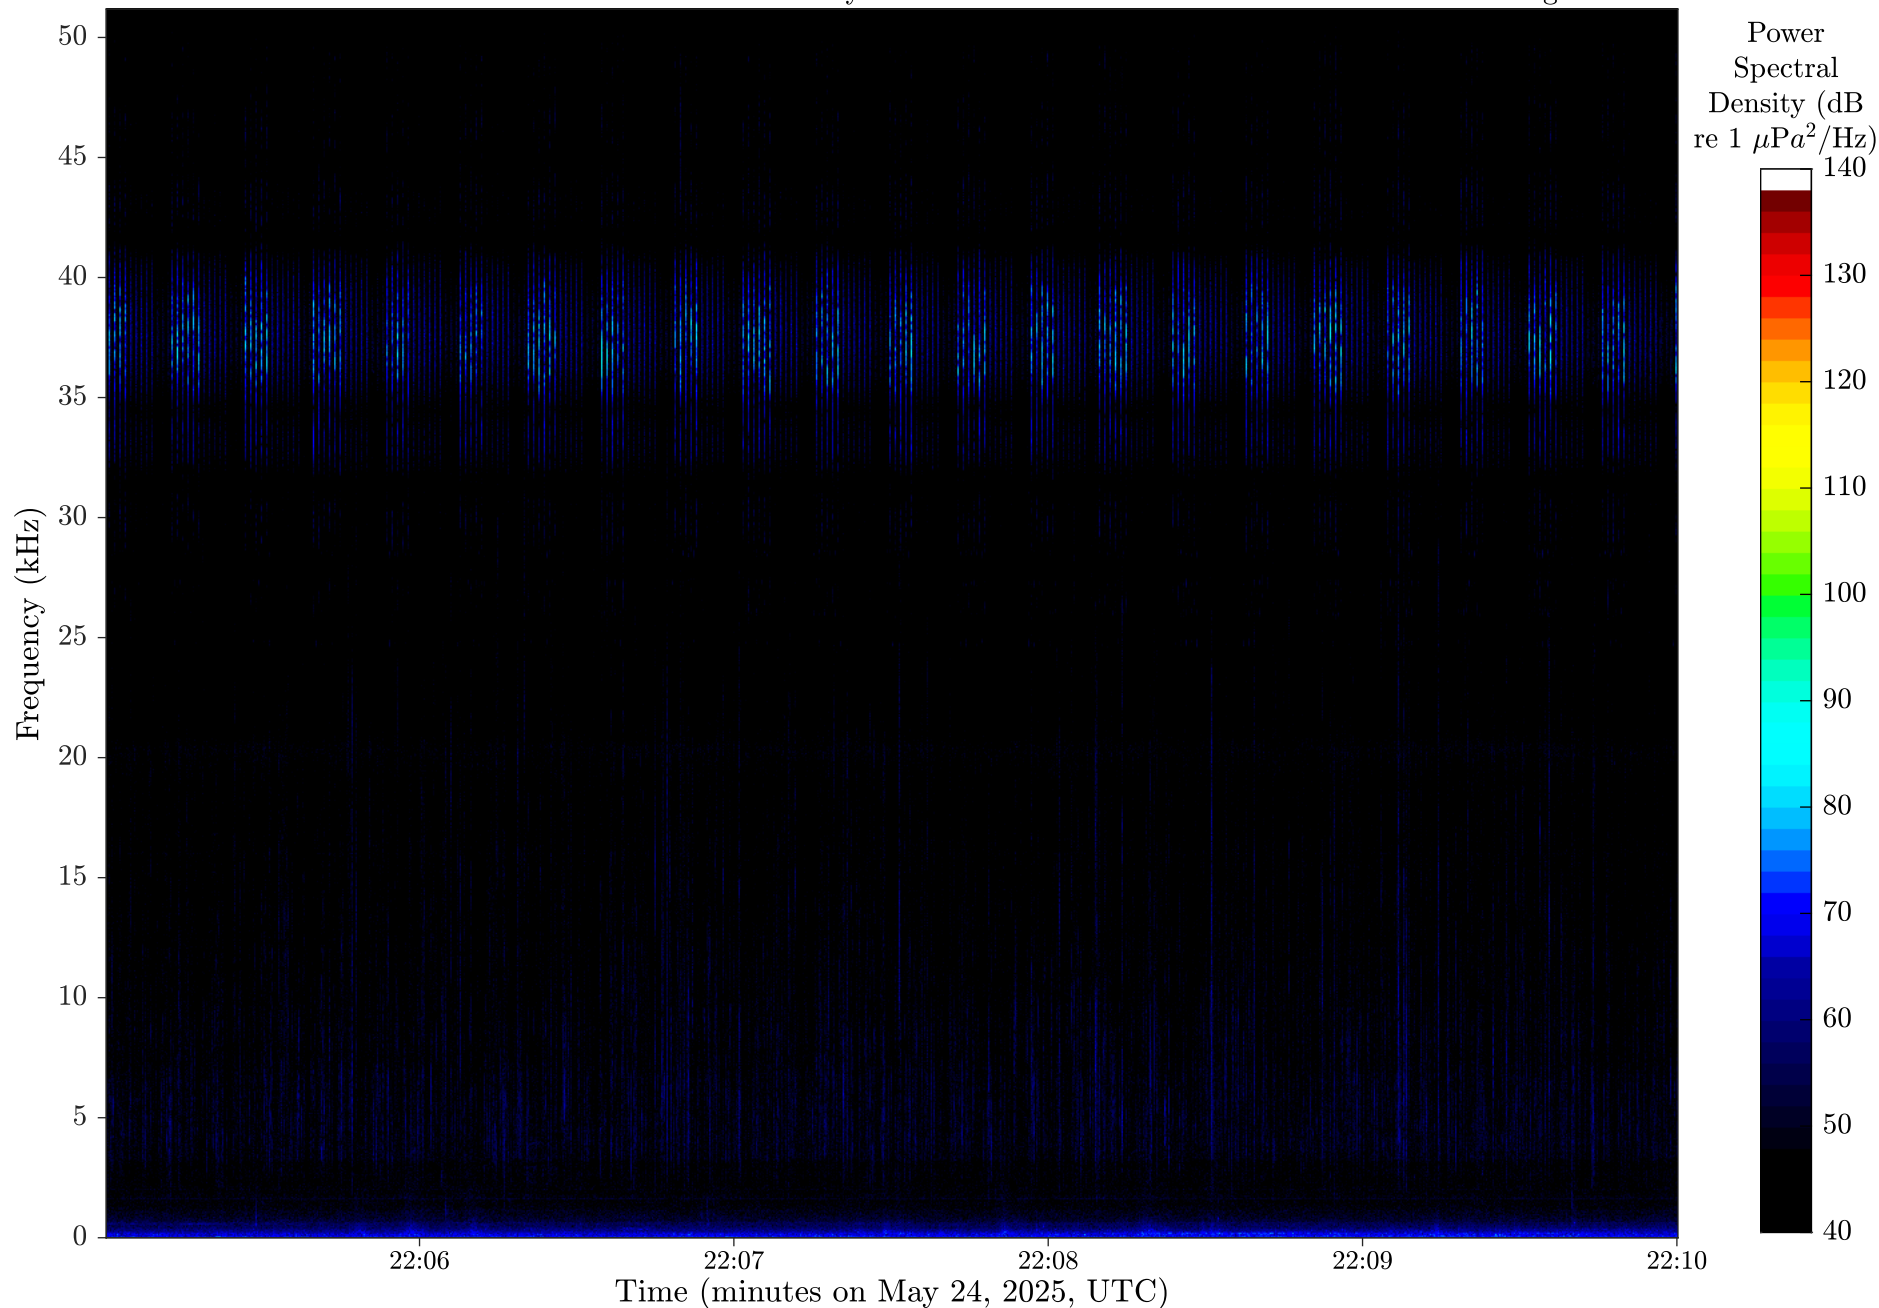


Comments: 34.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:43:20 UTC

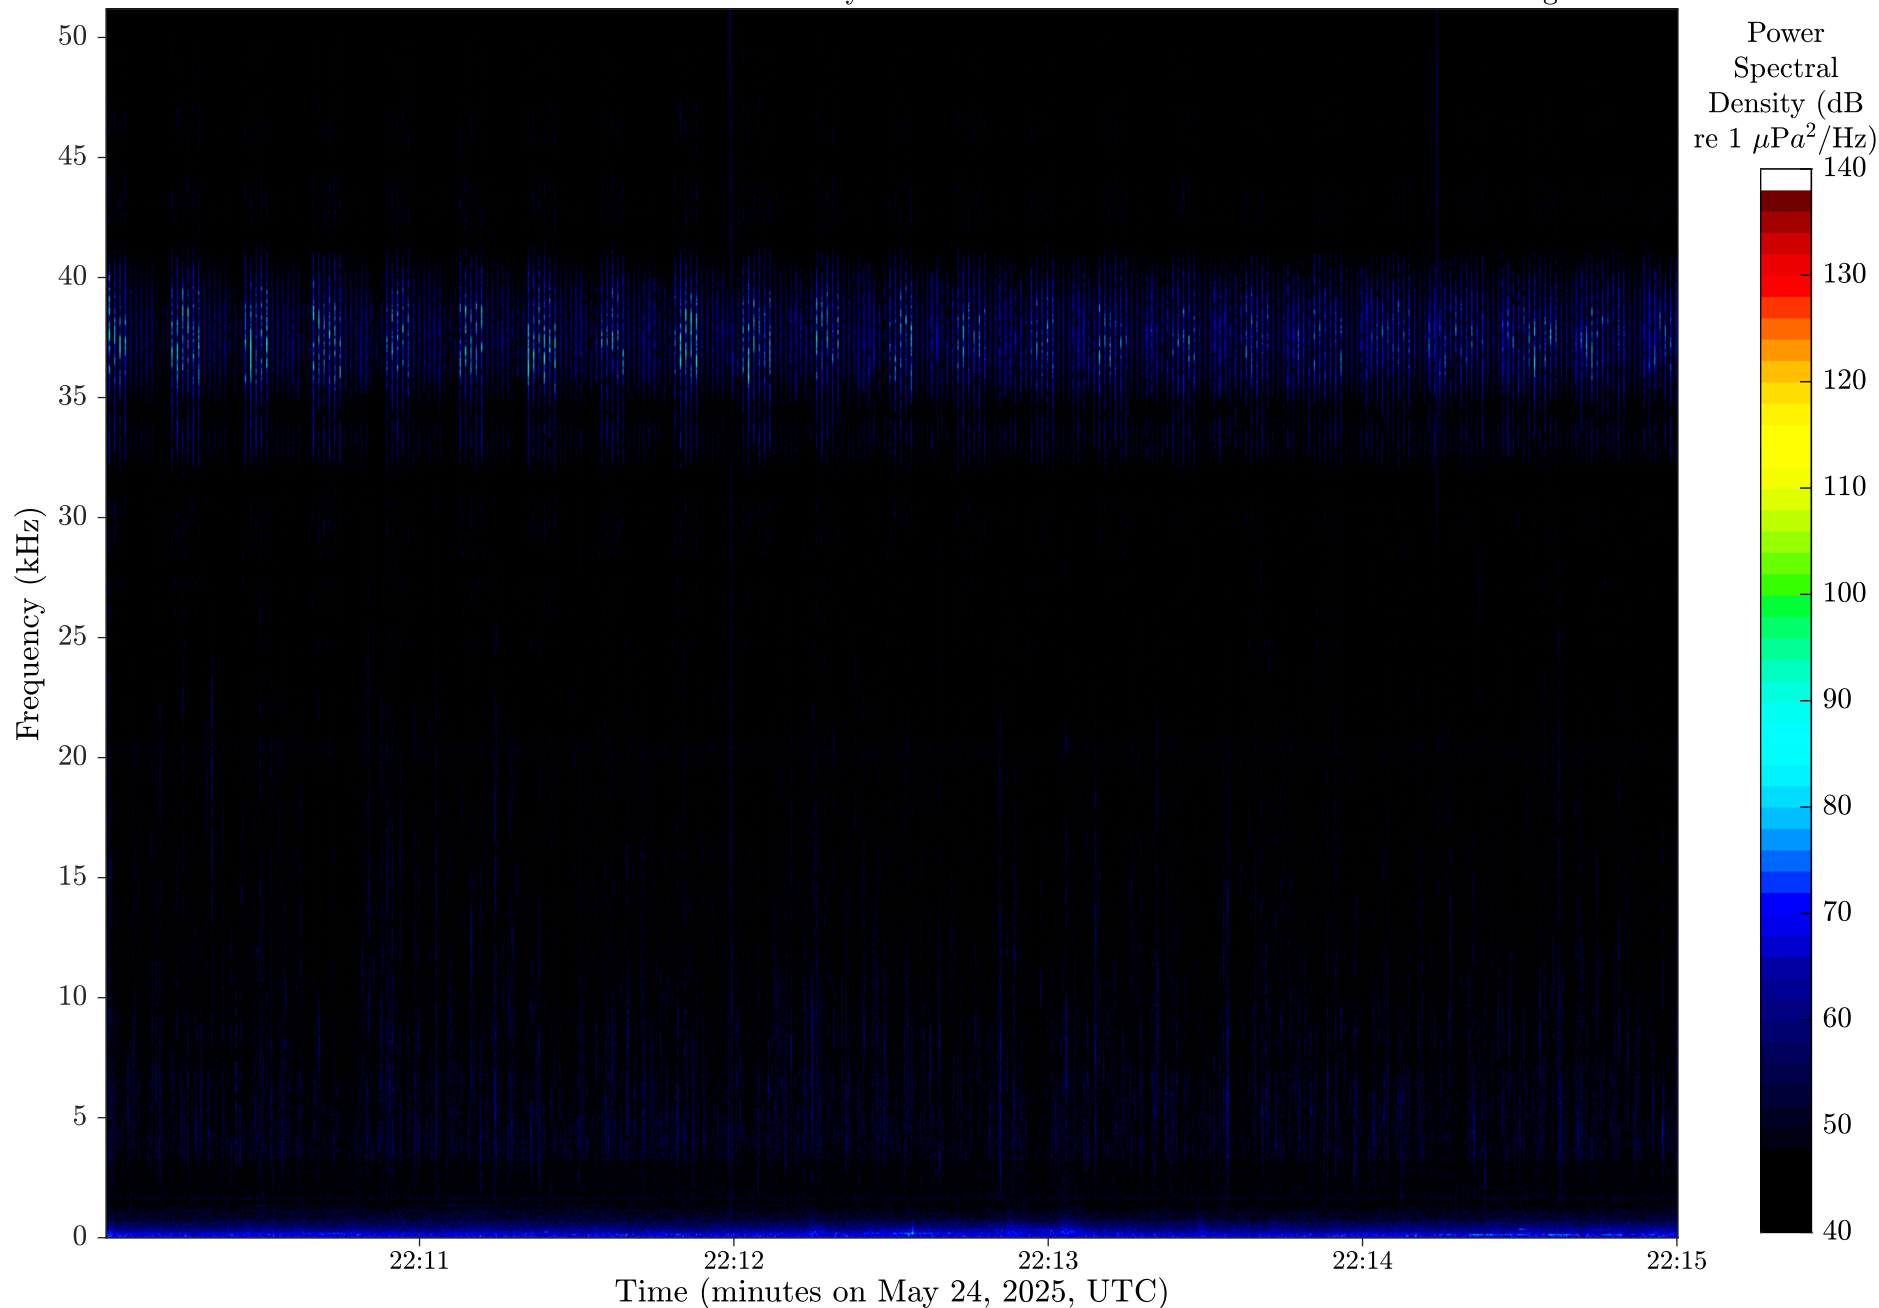

Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:43:28 UTC

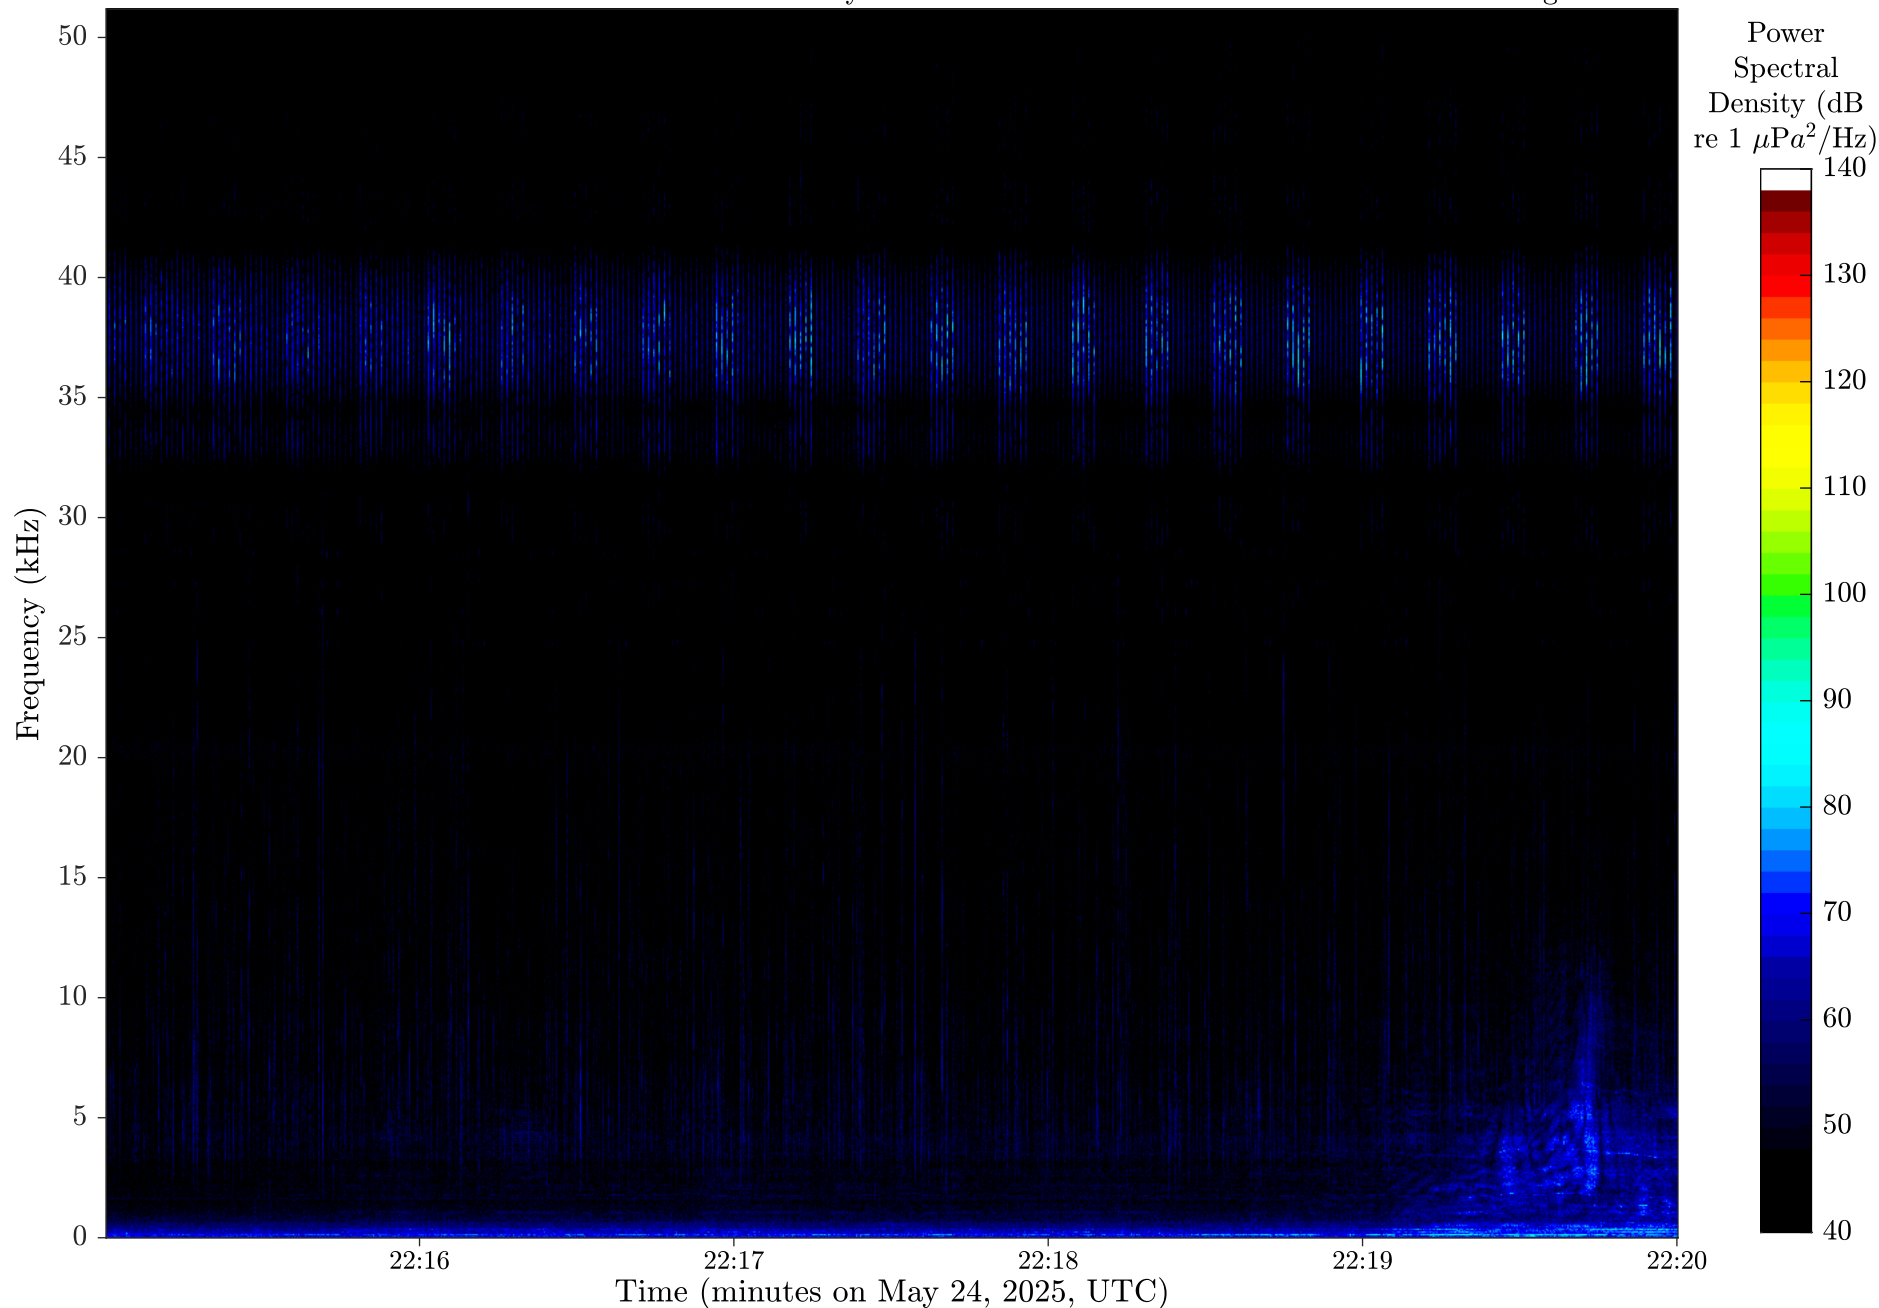

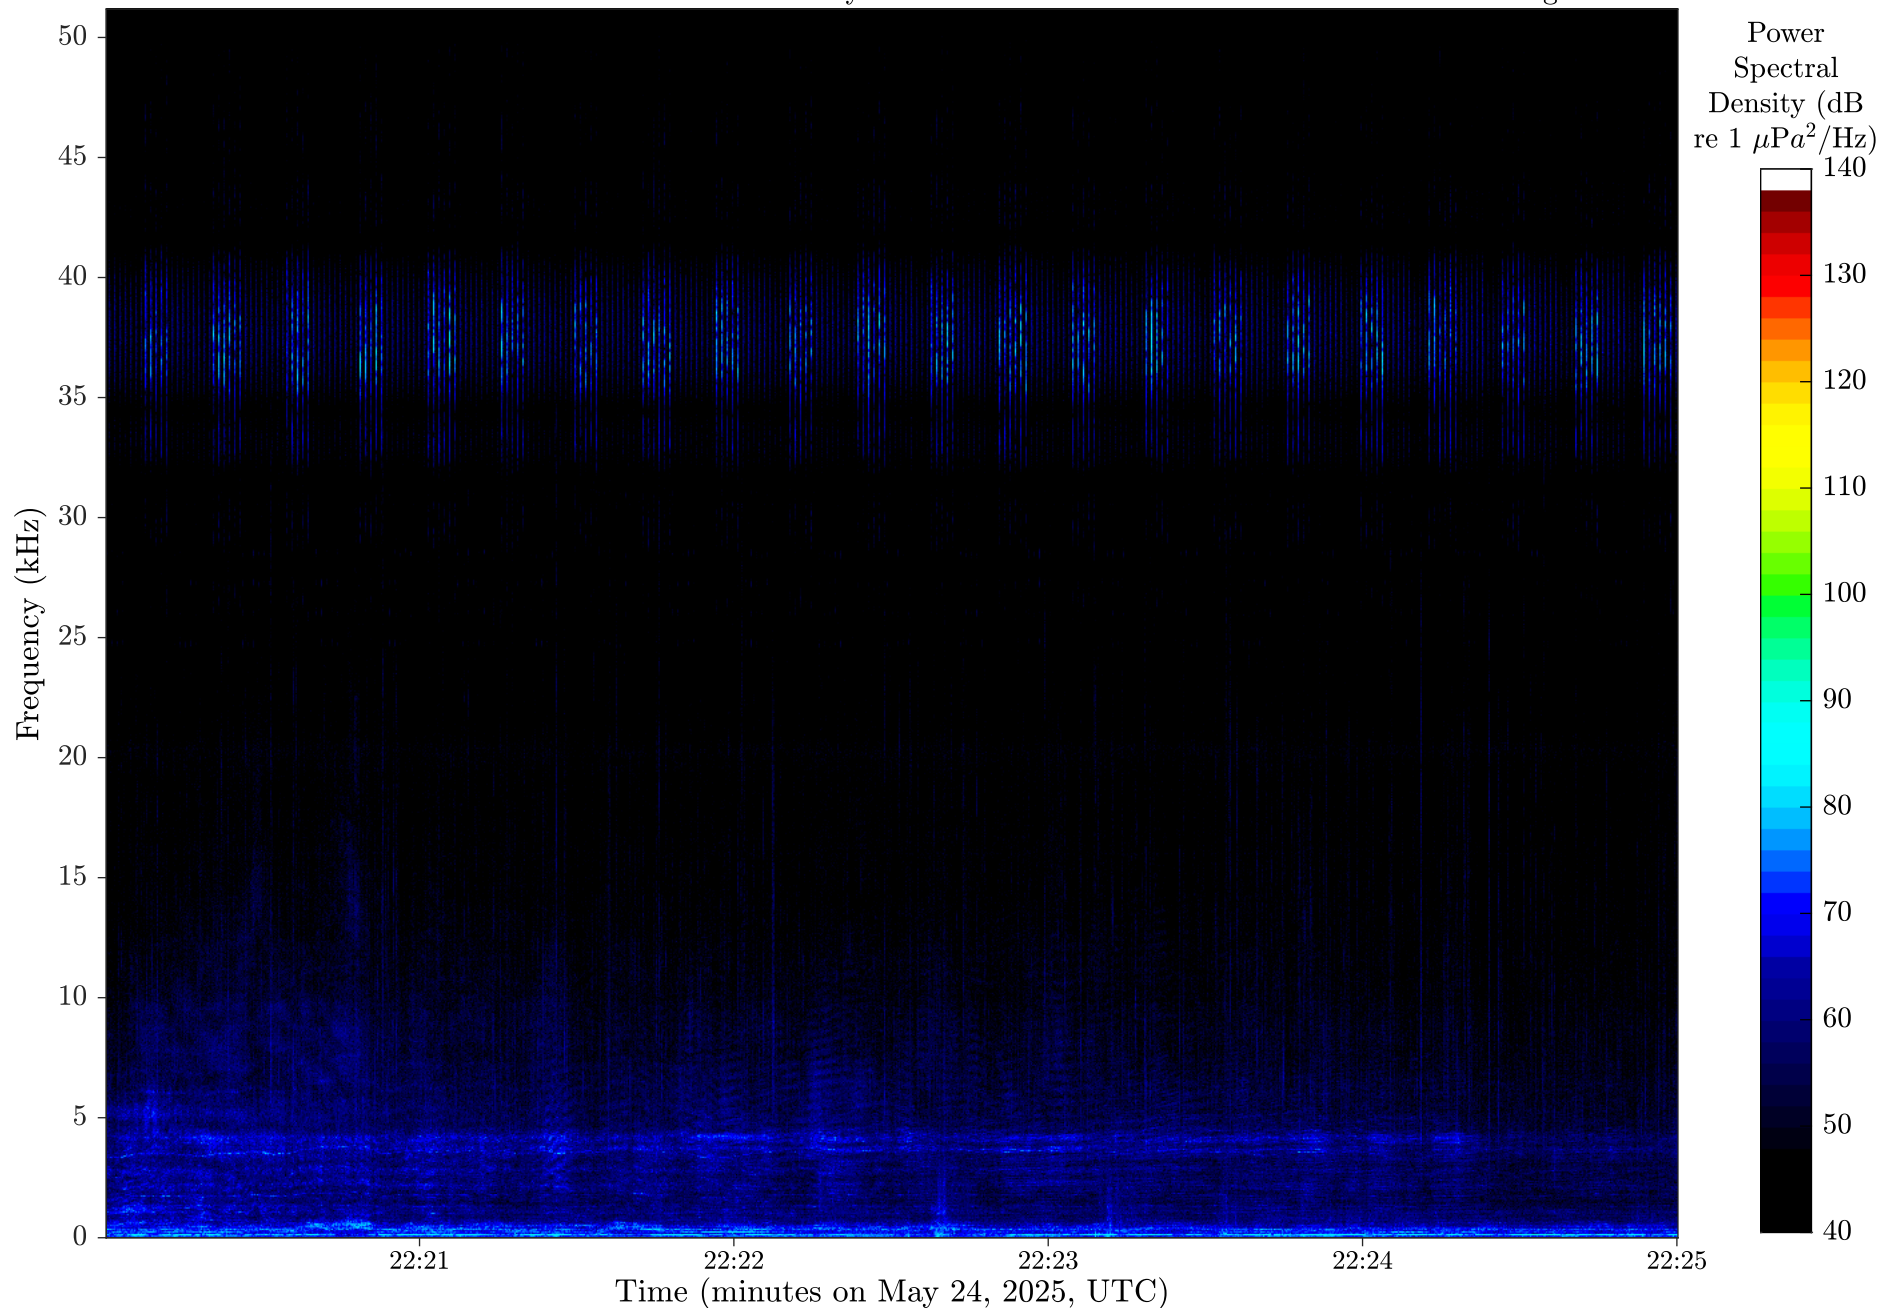


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:43:44 UTC

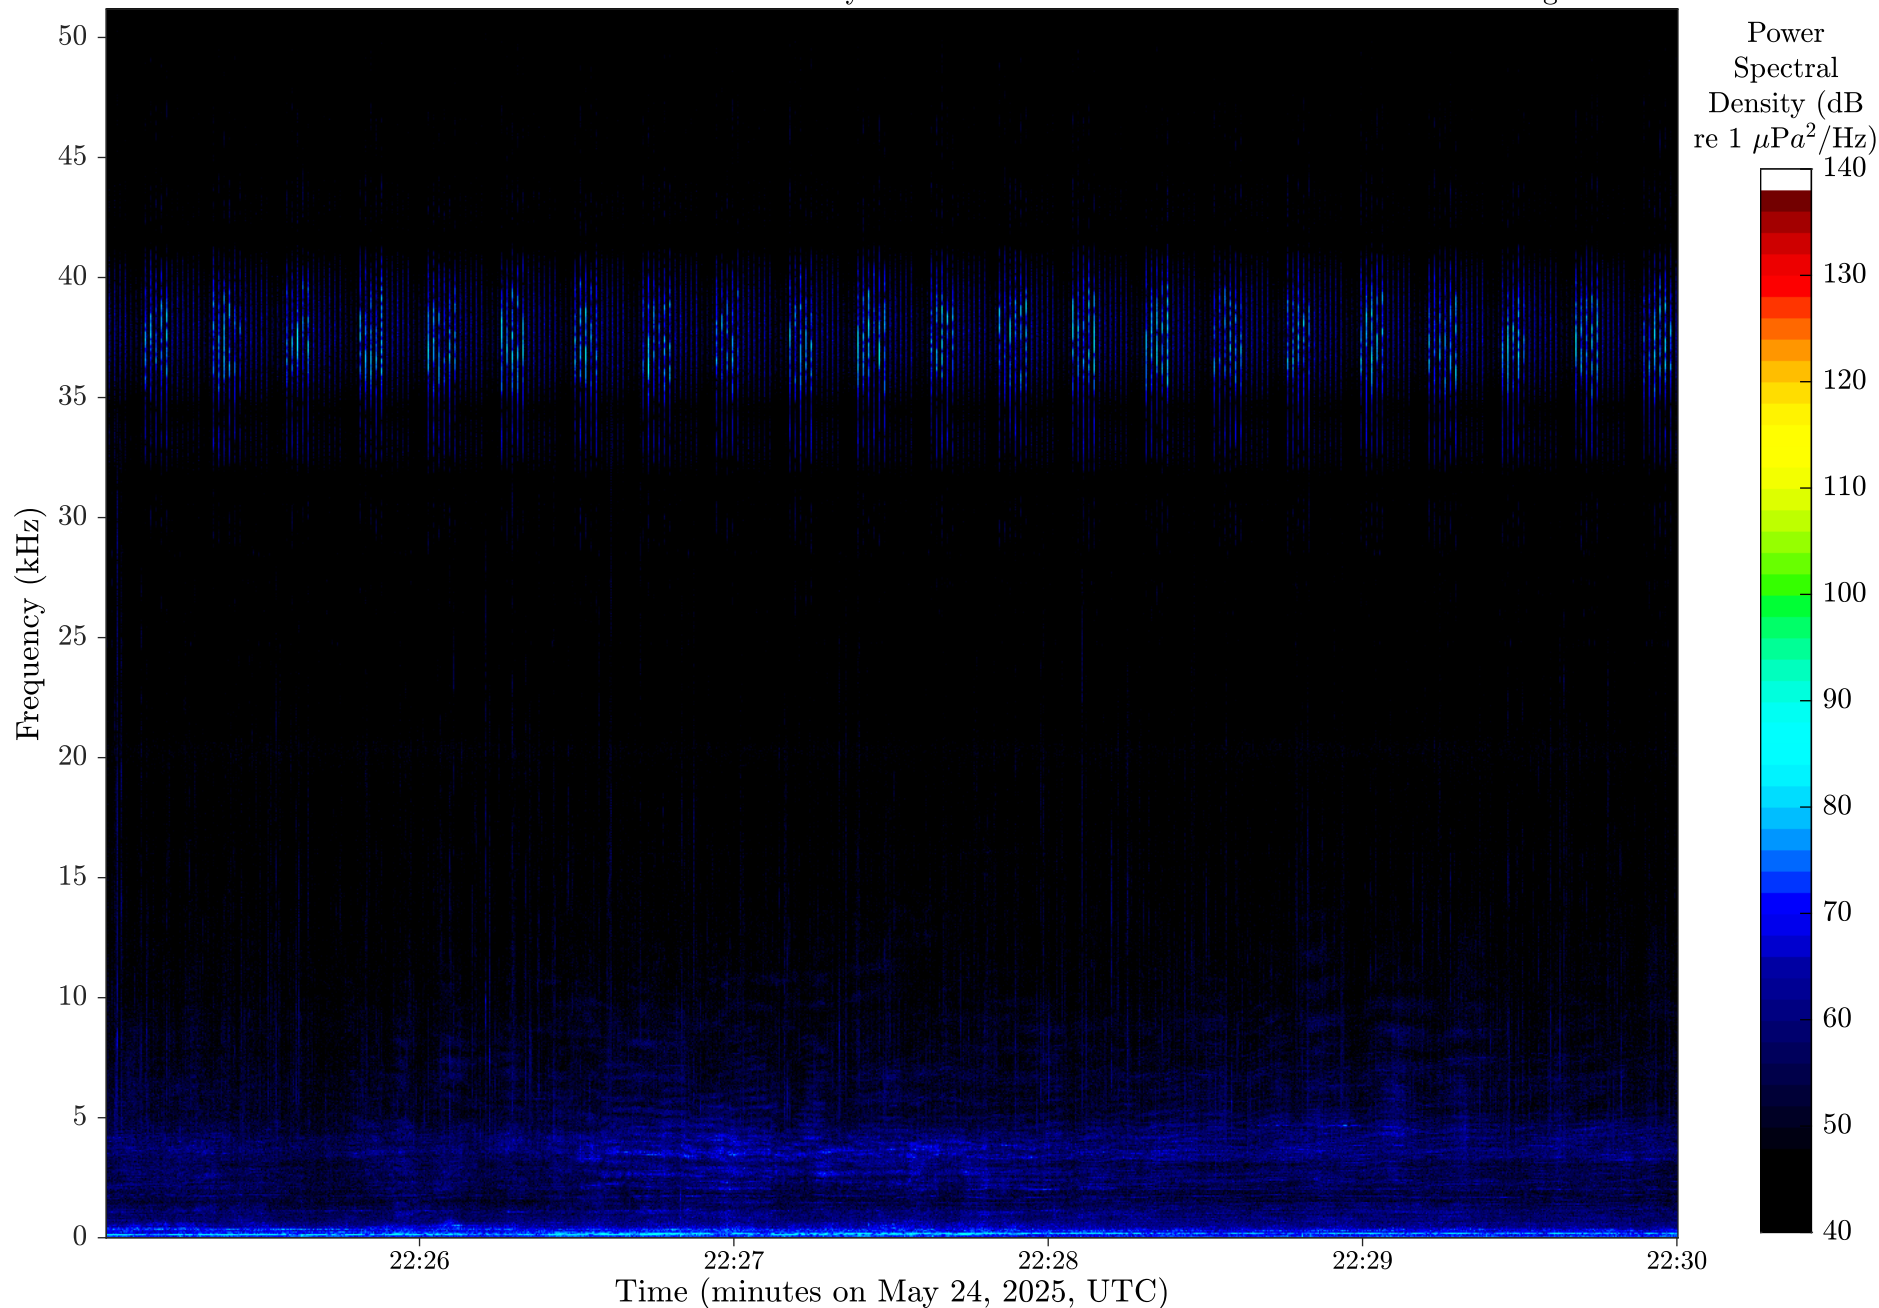


Comments: 34.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:43:51 UTC

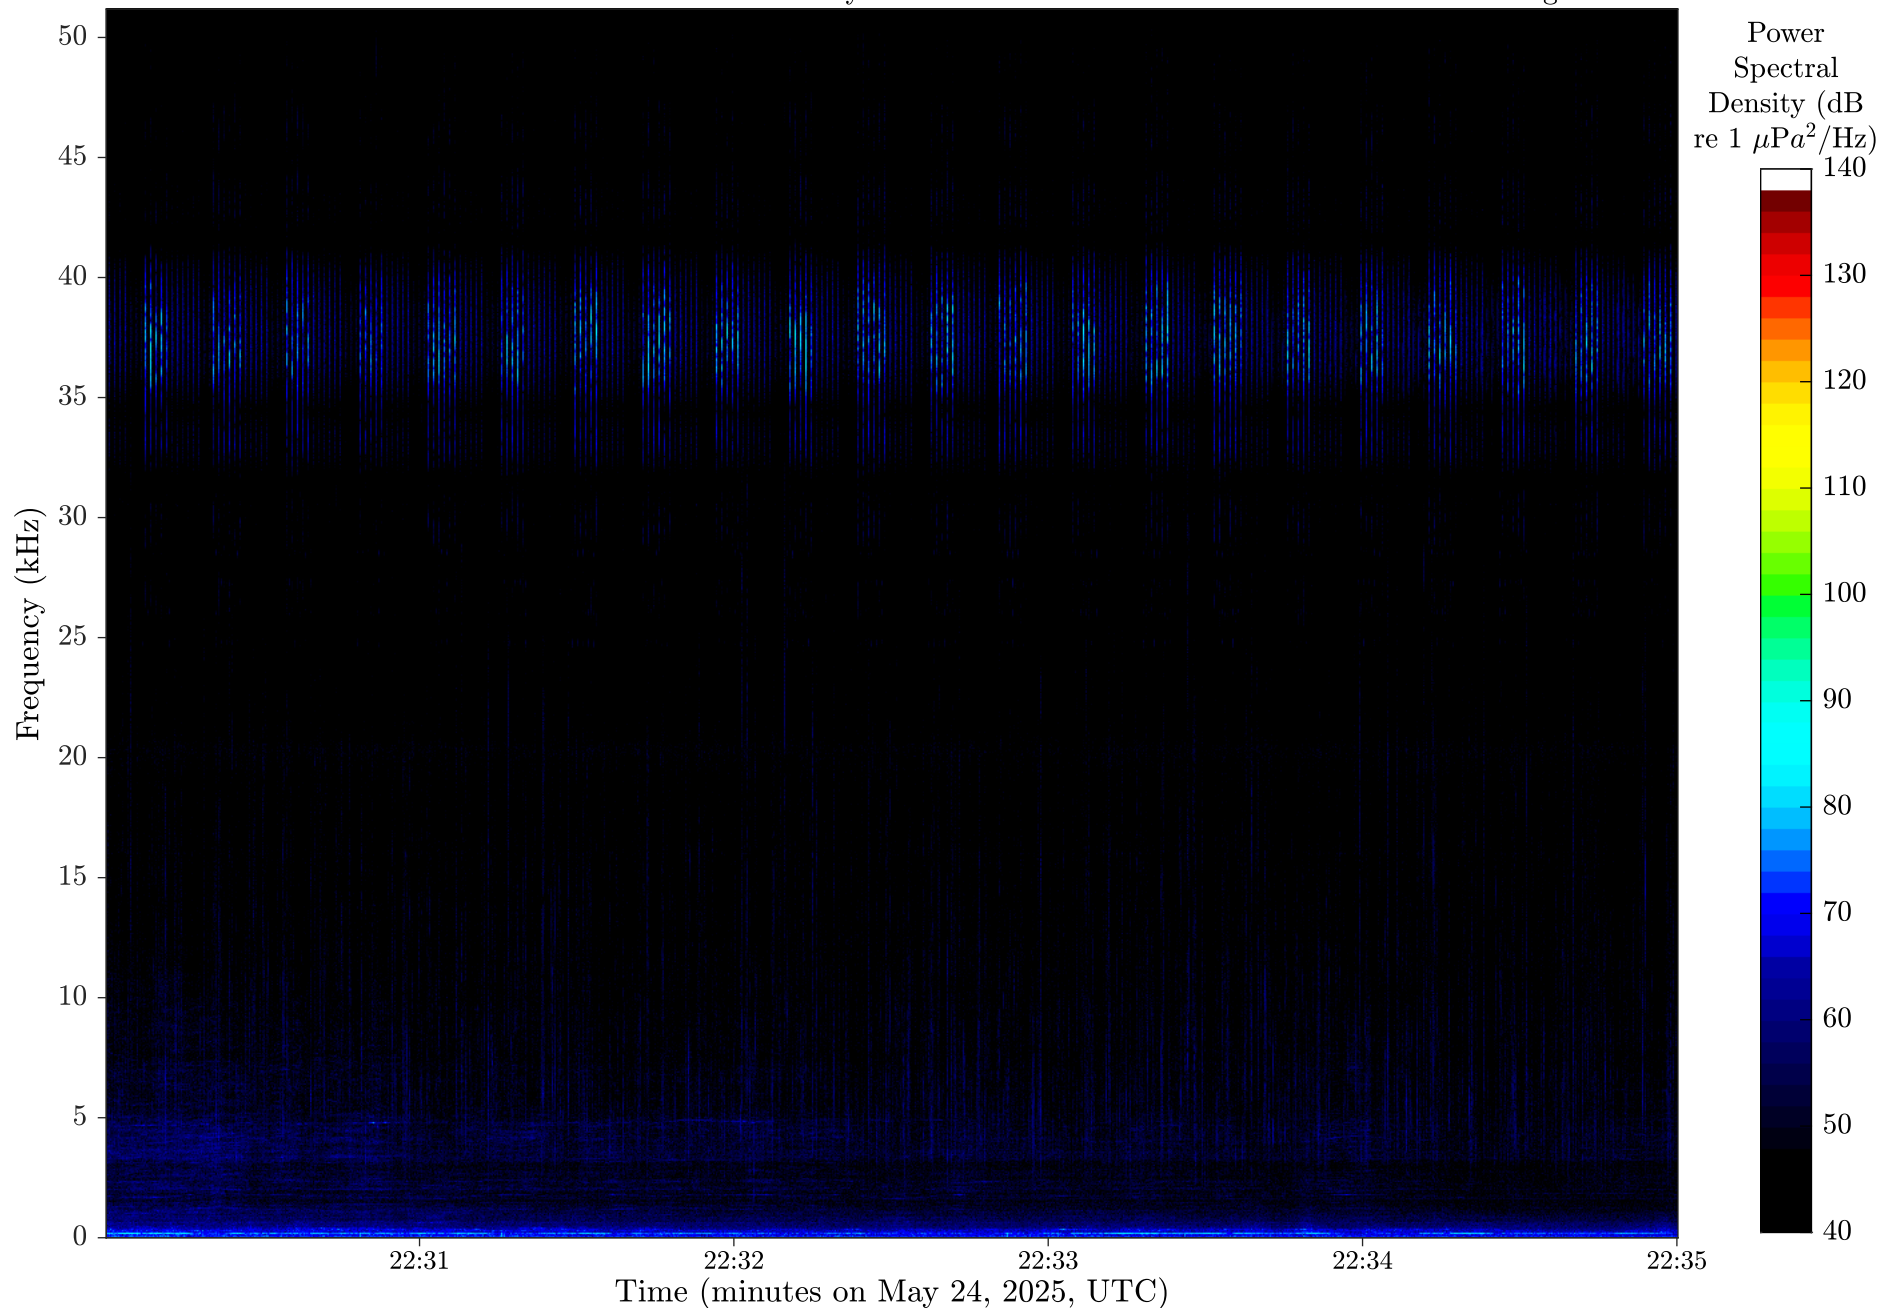


Comments: 34.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:43:59 UTC

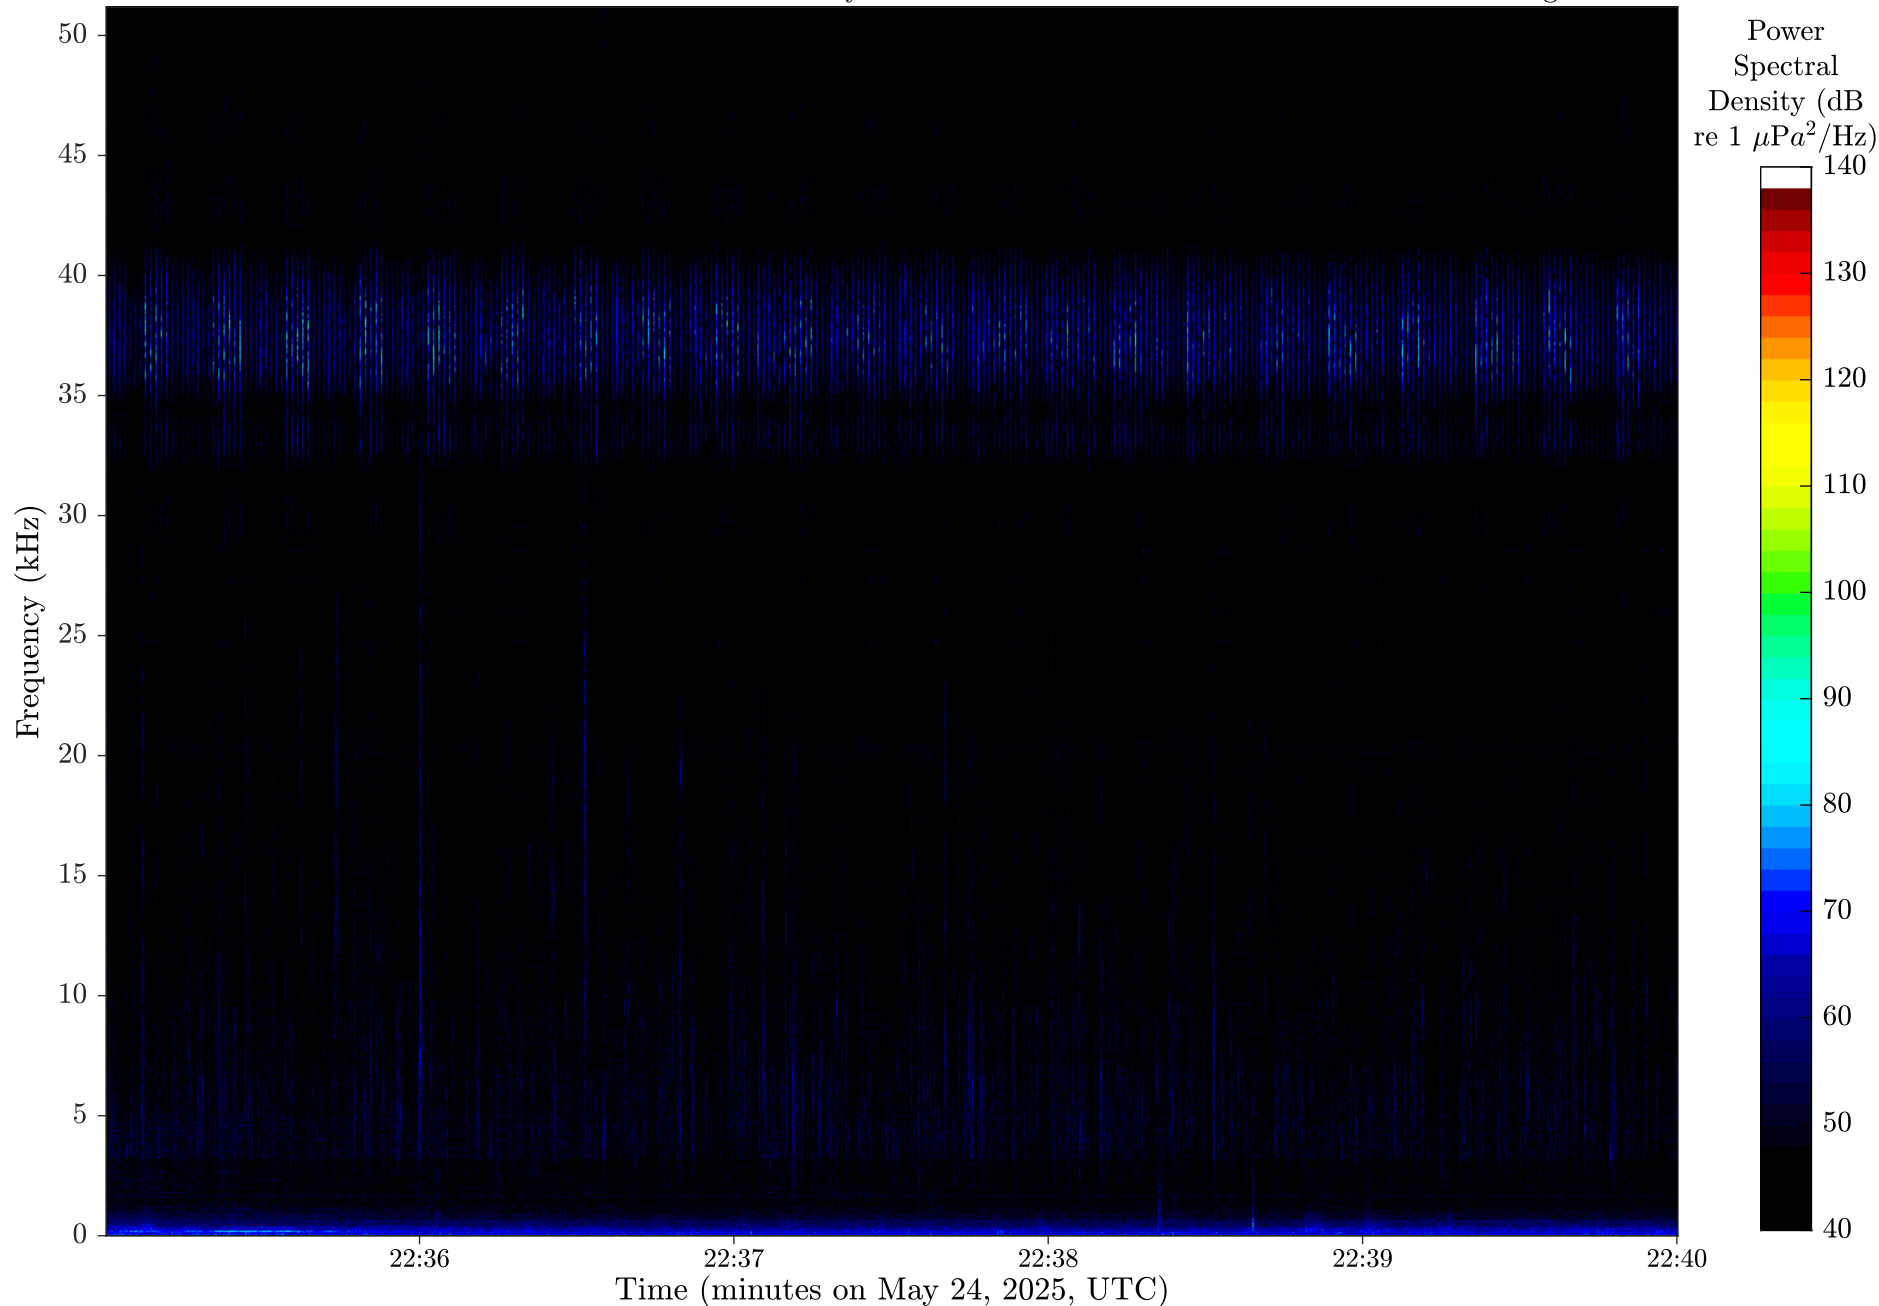


Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:07 UTC

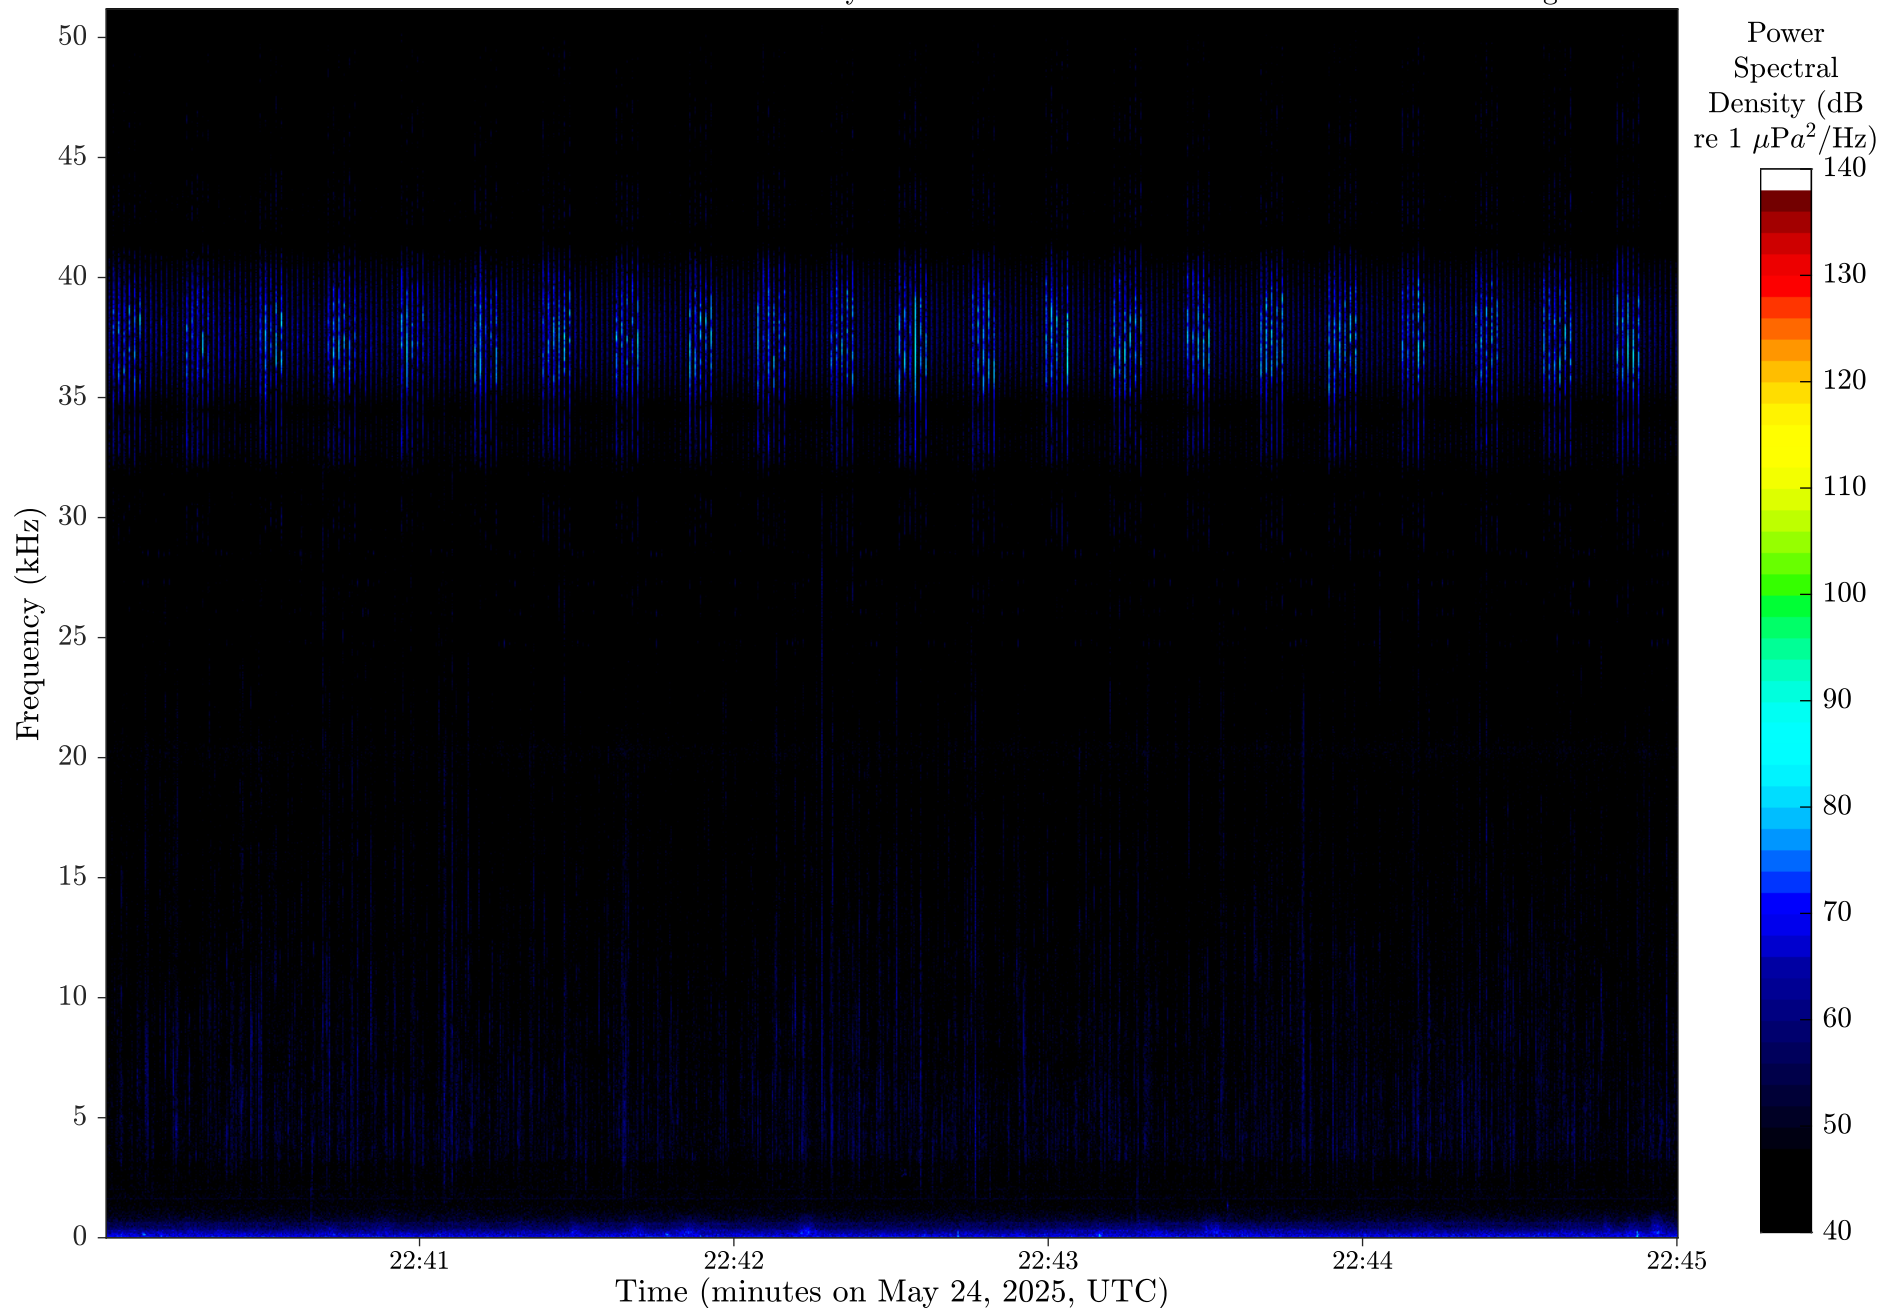


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:15 UTC

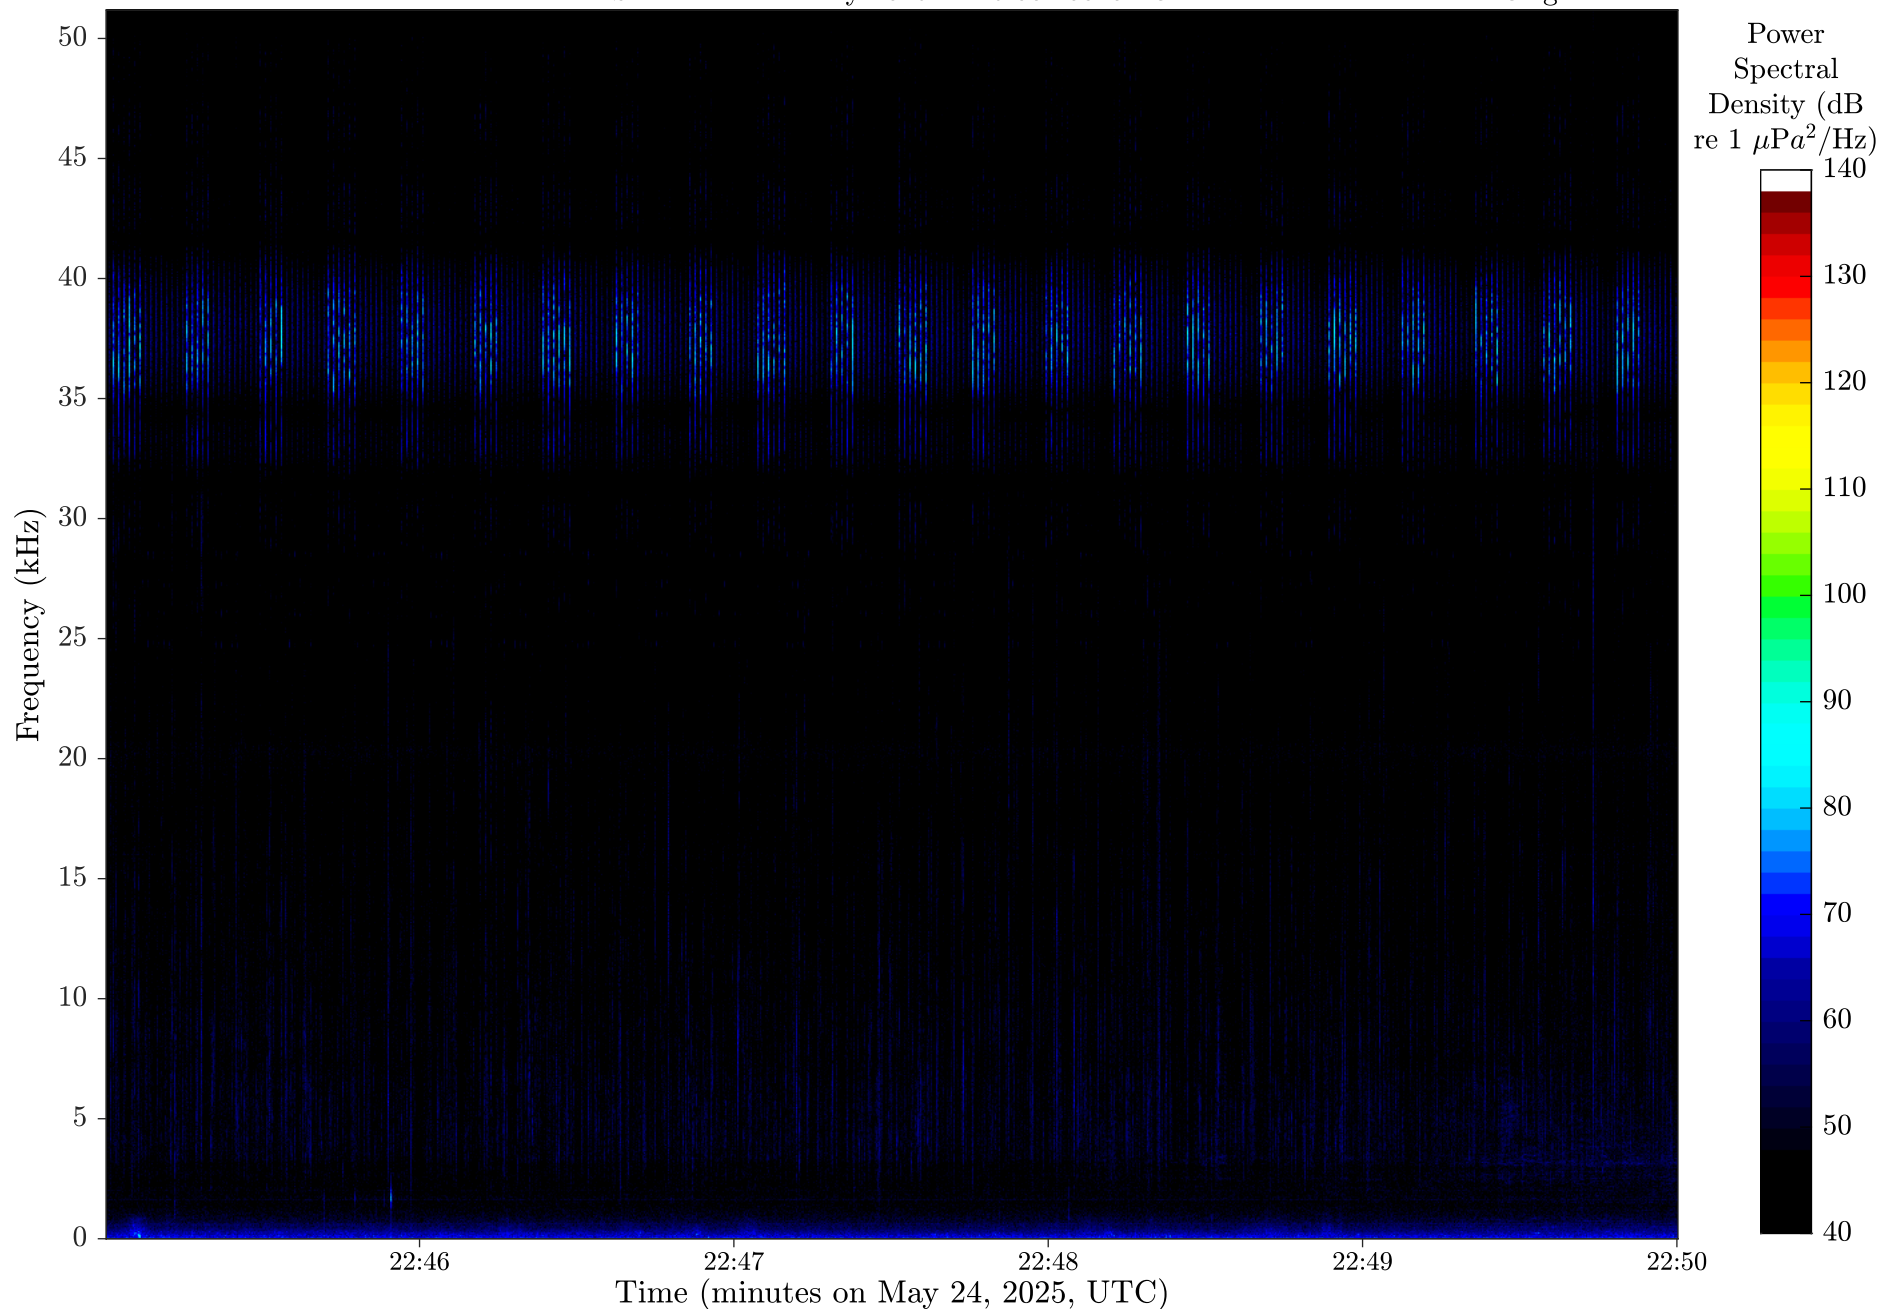


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:22 UTC

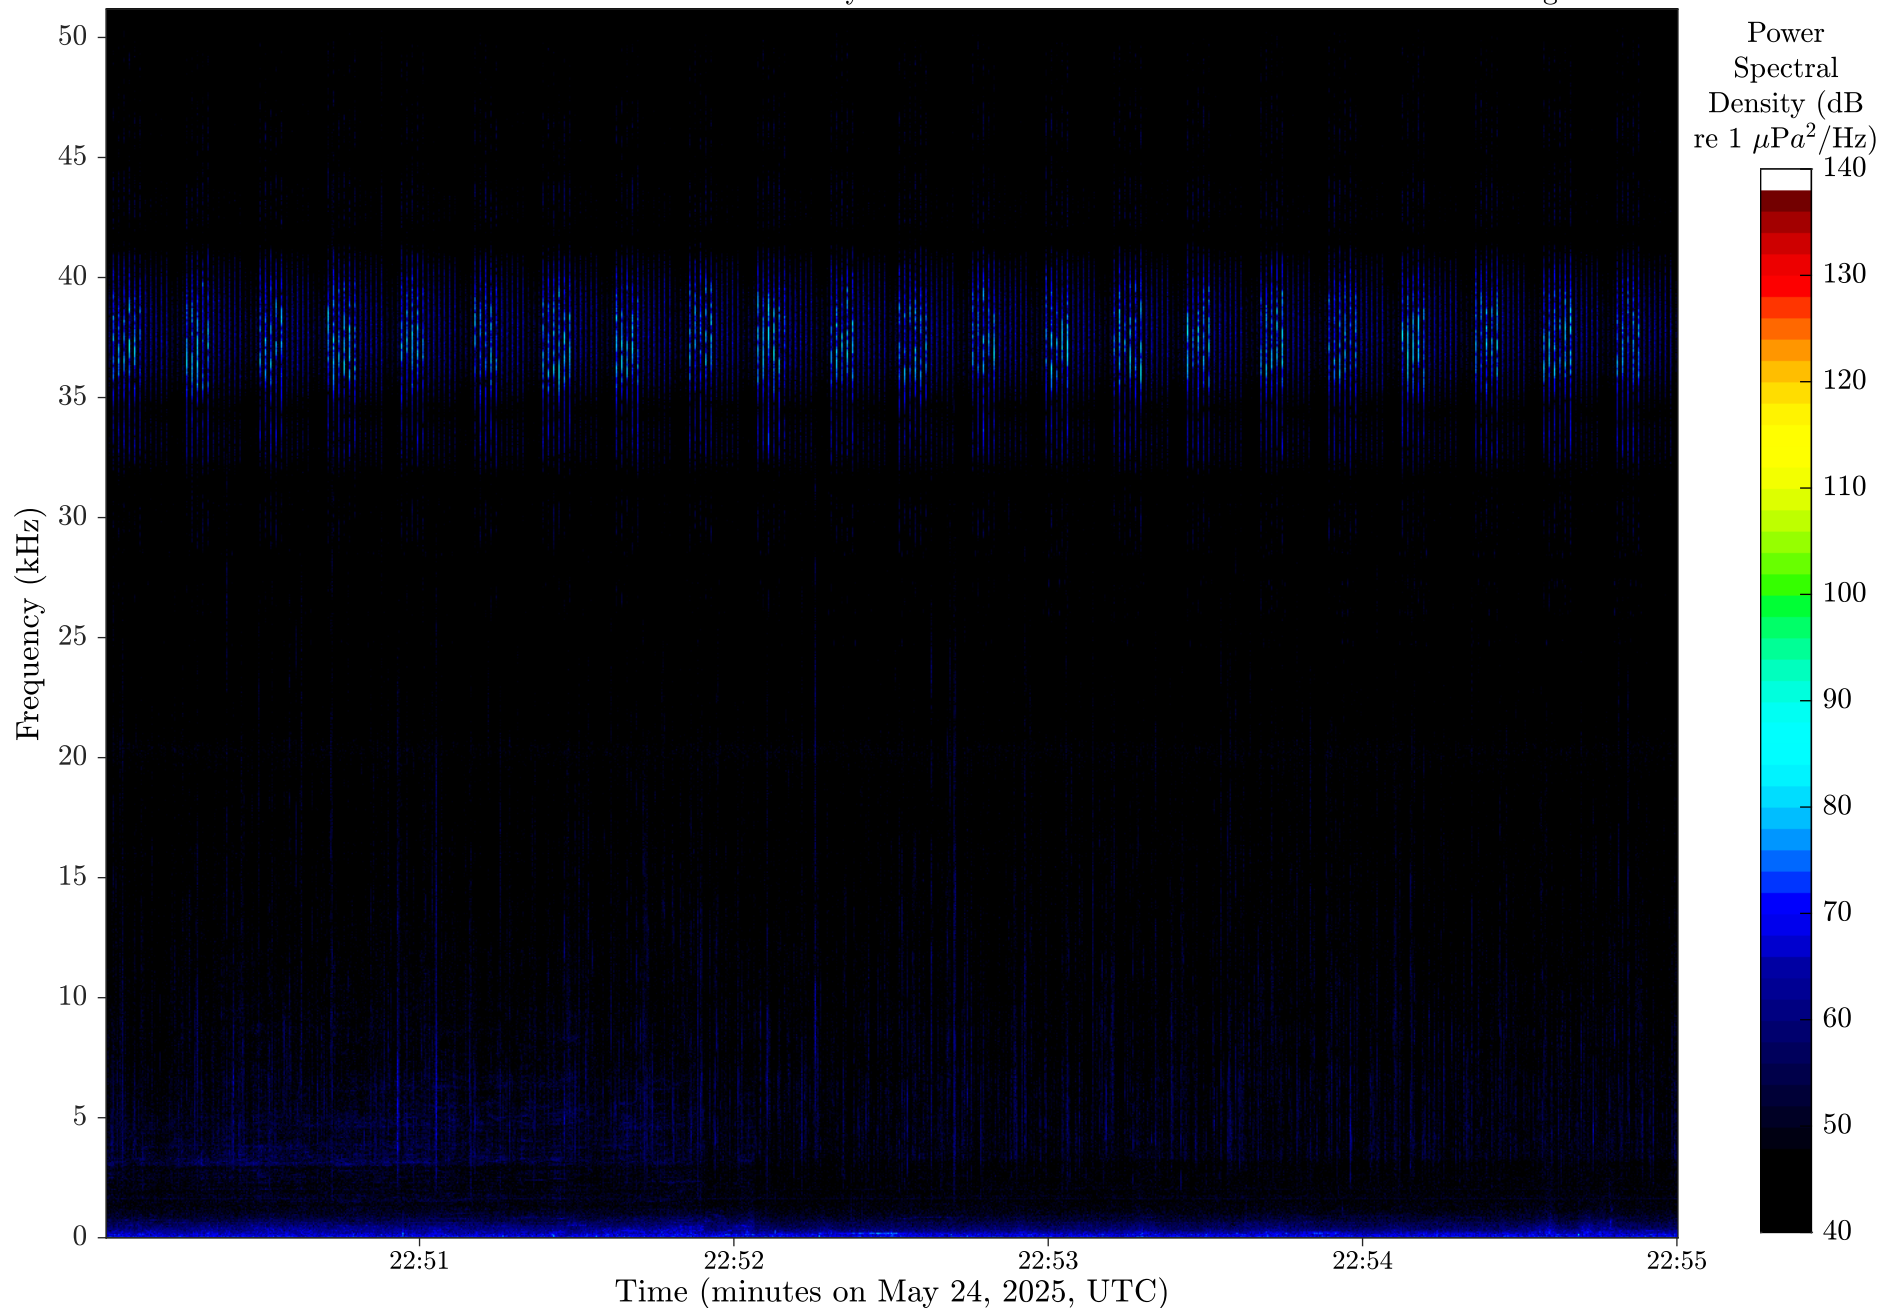


Comments: 34.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:29 UTC

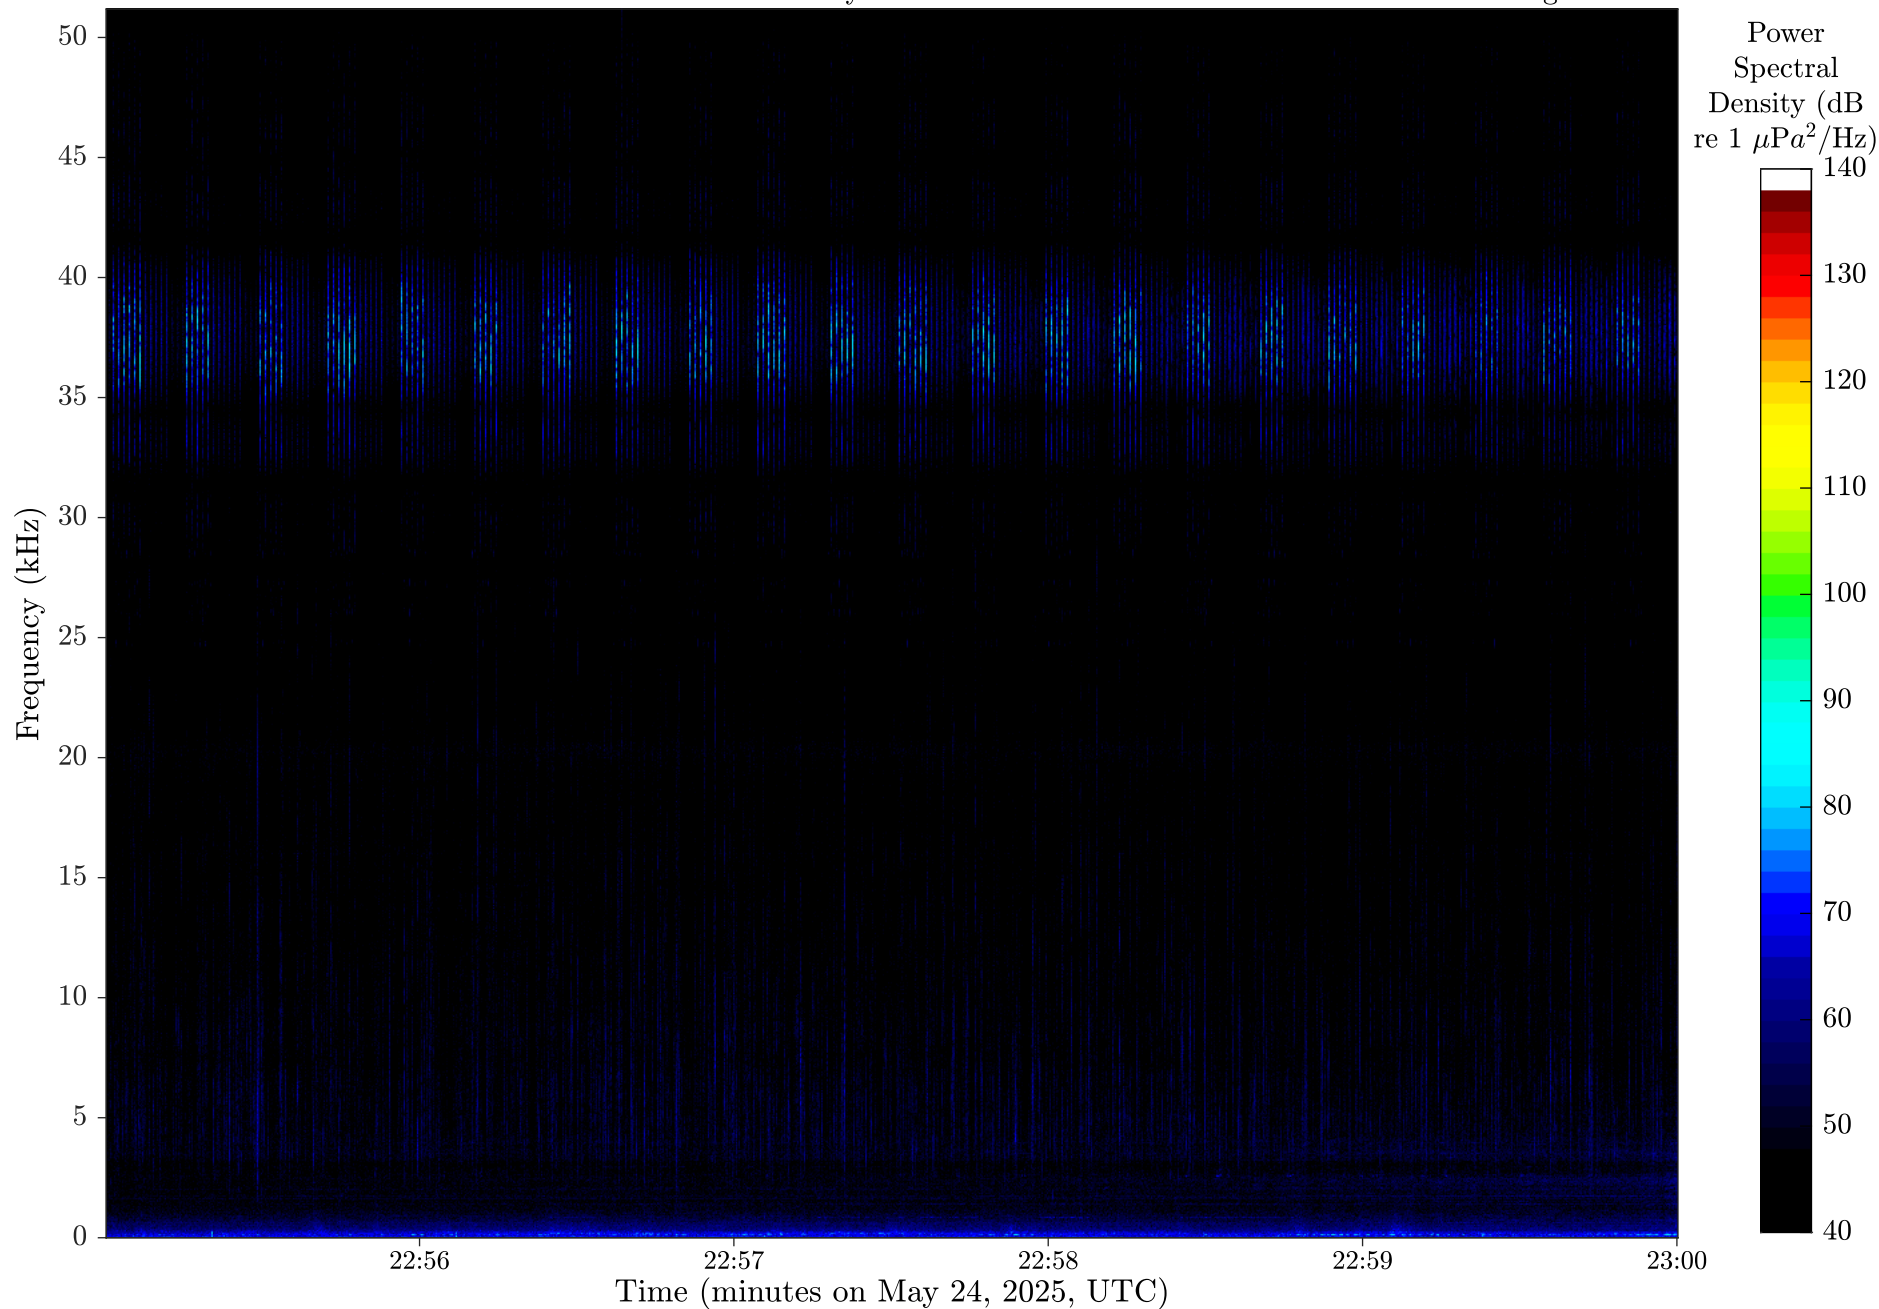


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:37 UTC

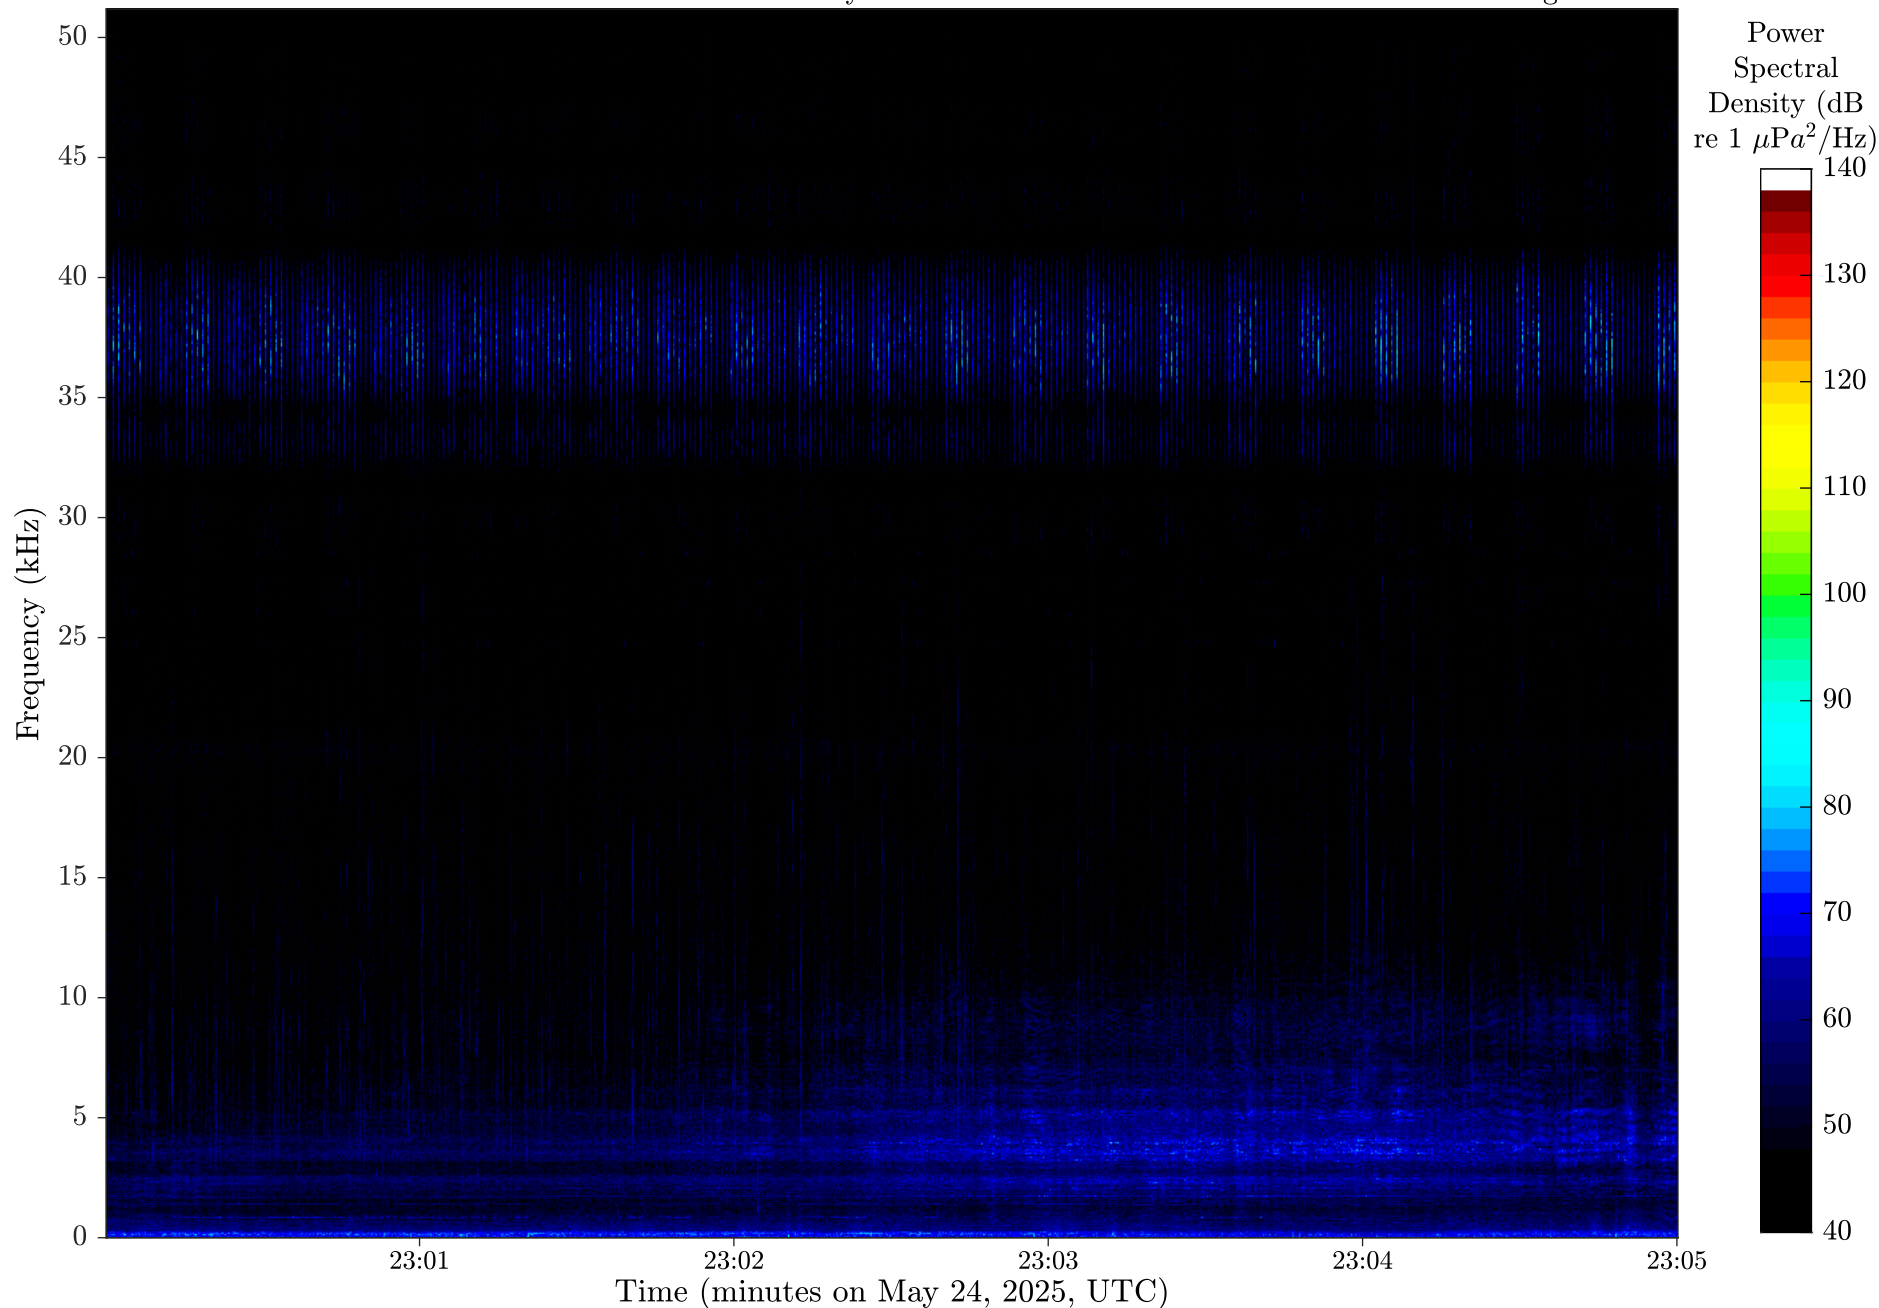


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:44 UTC

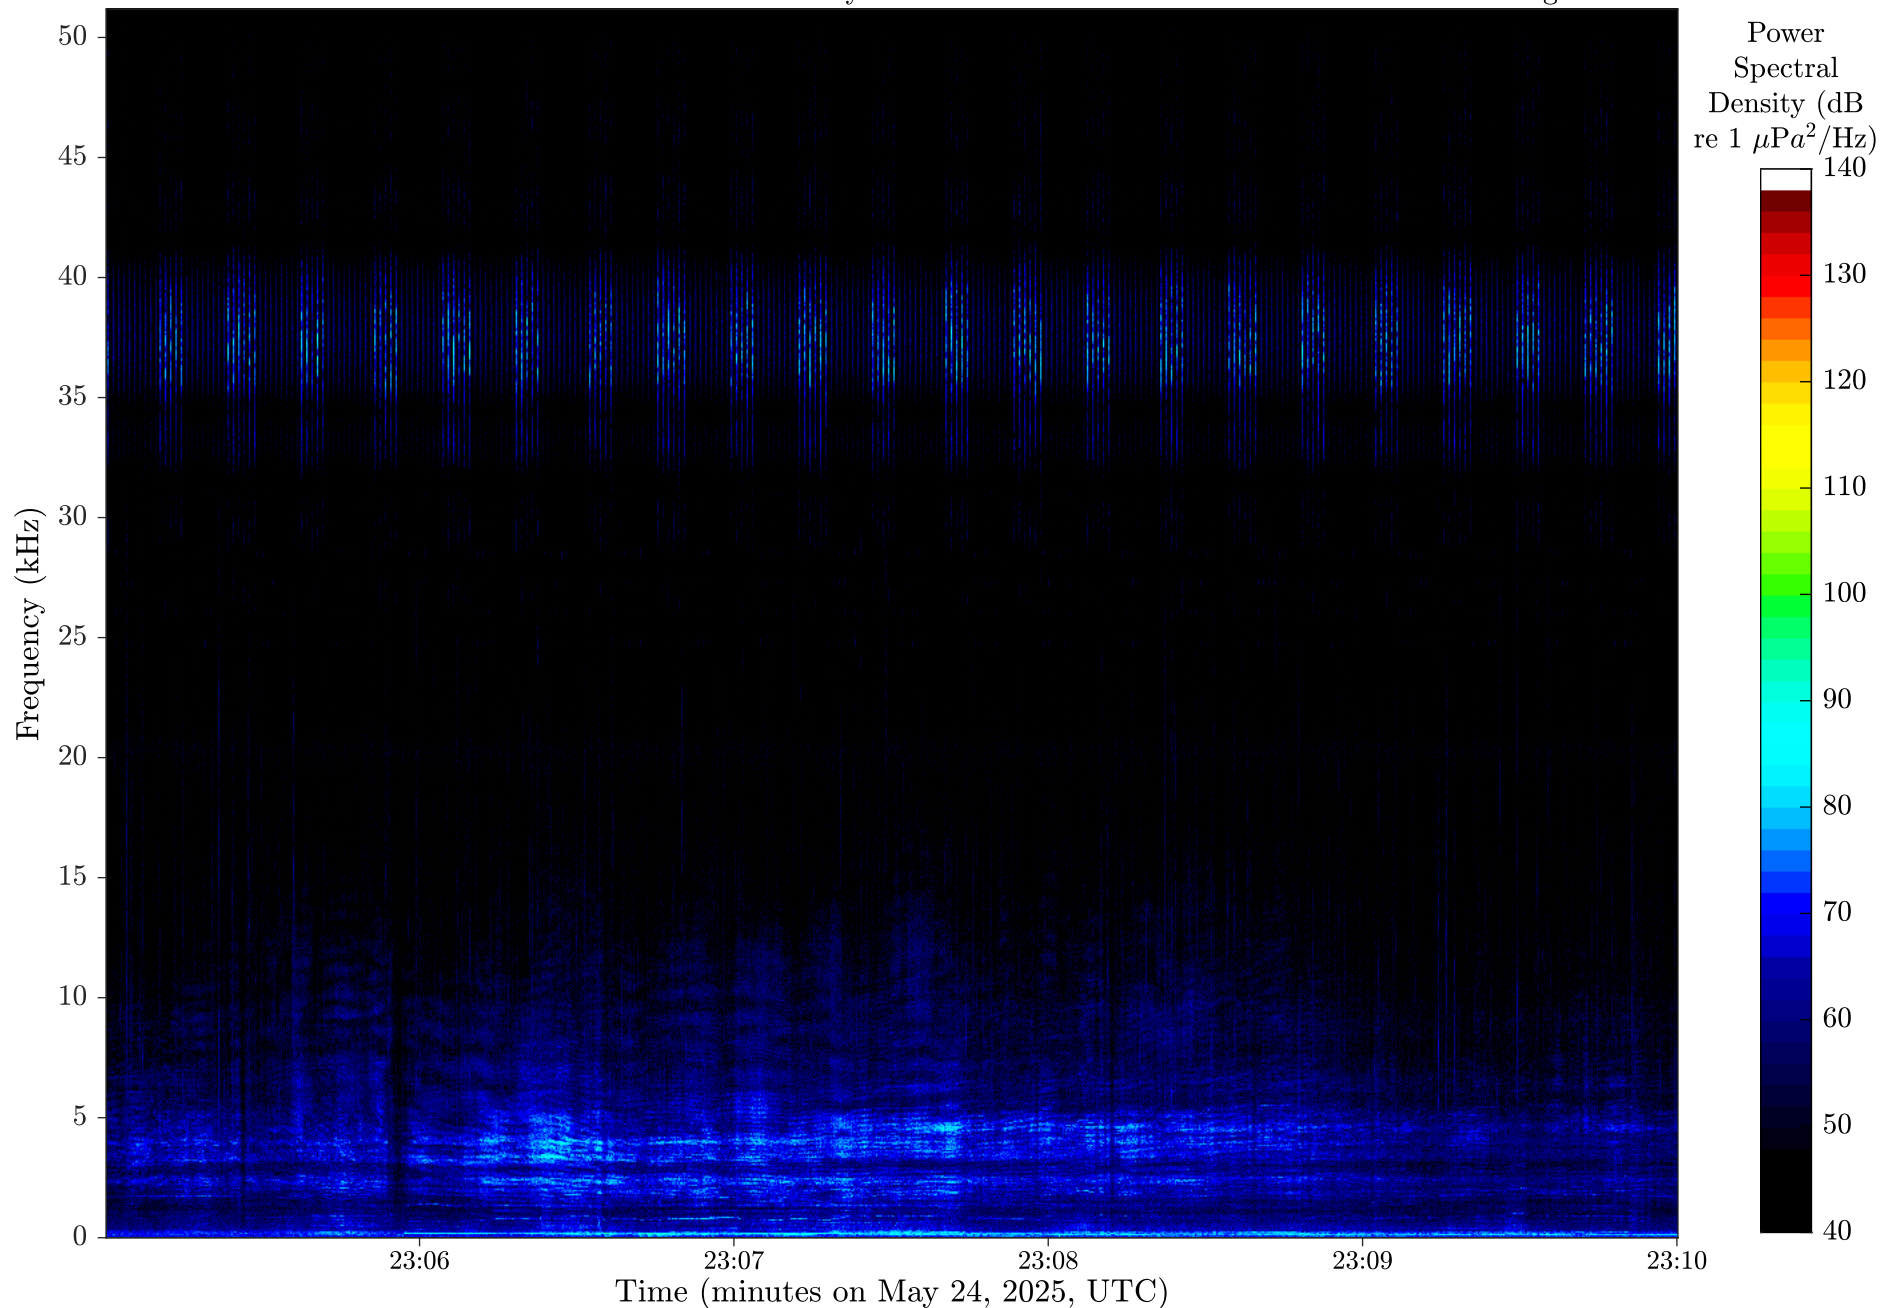


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:51 UTC

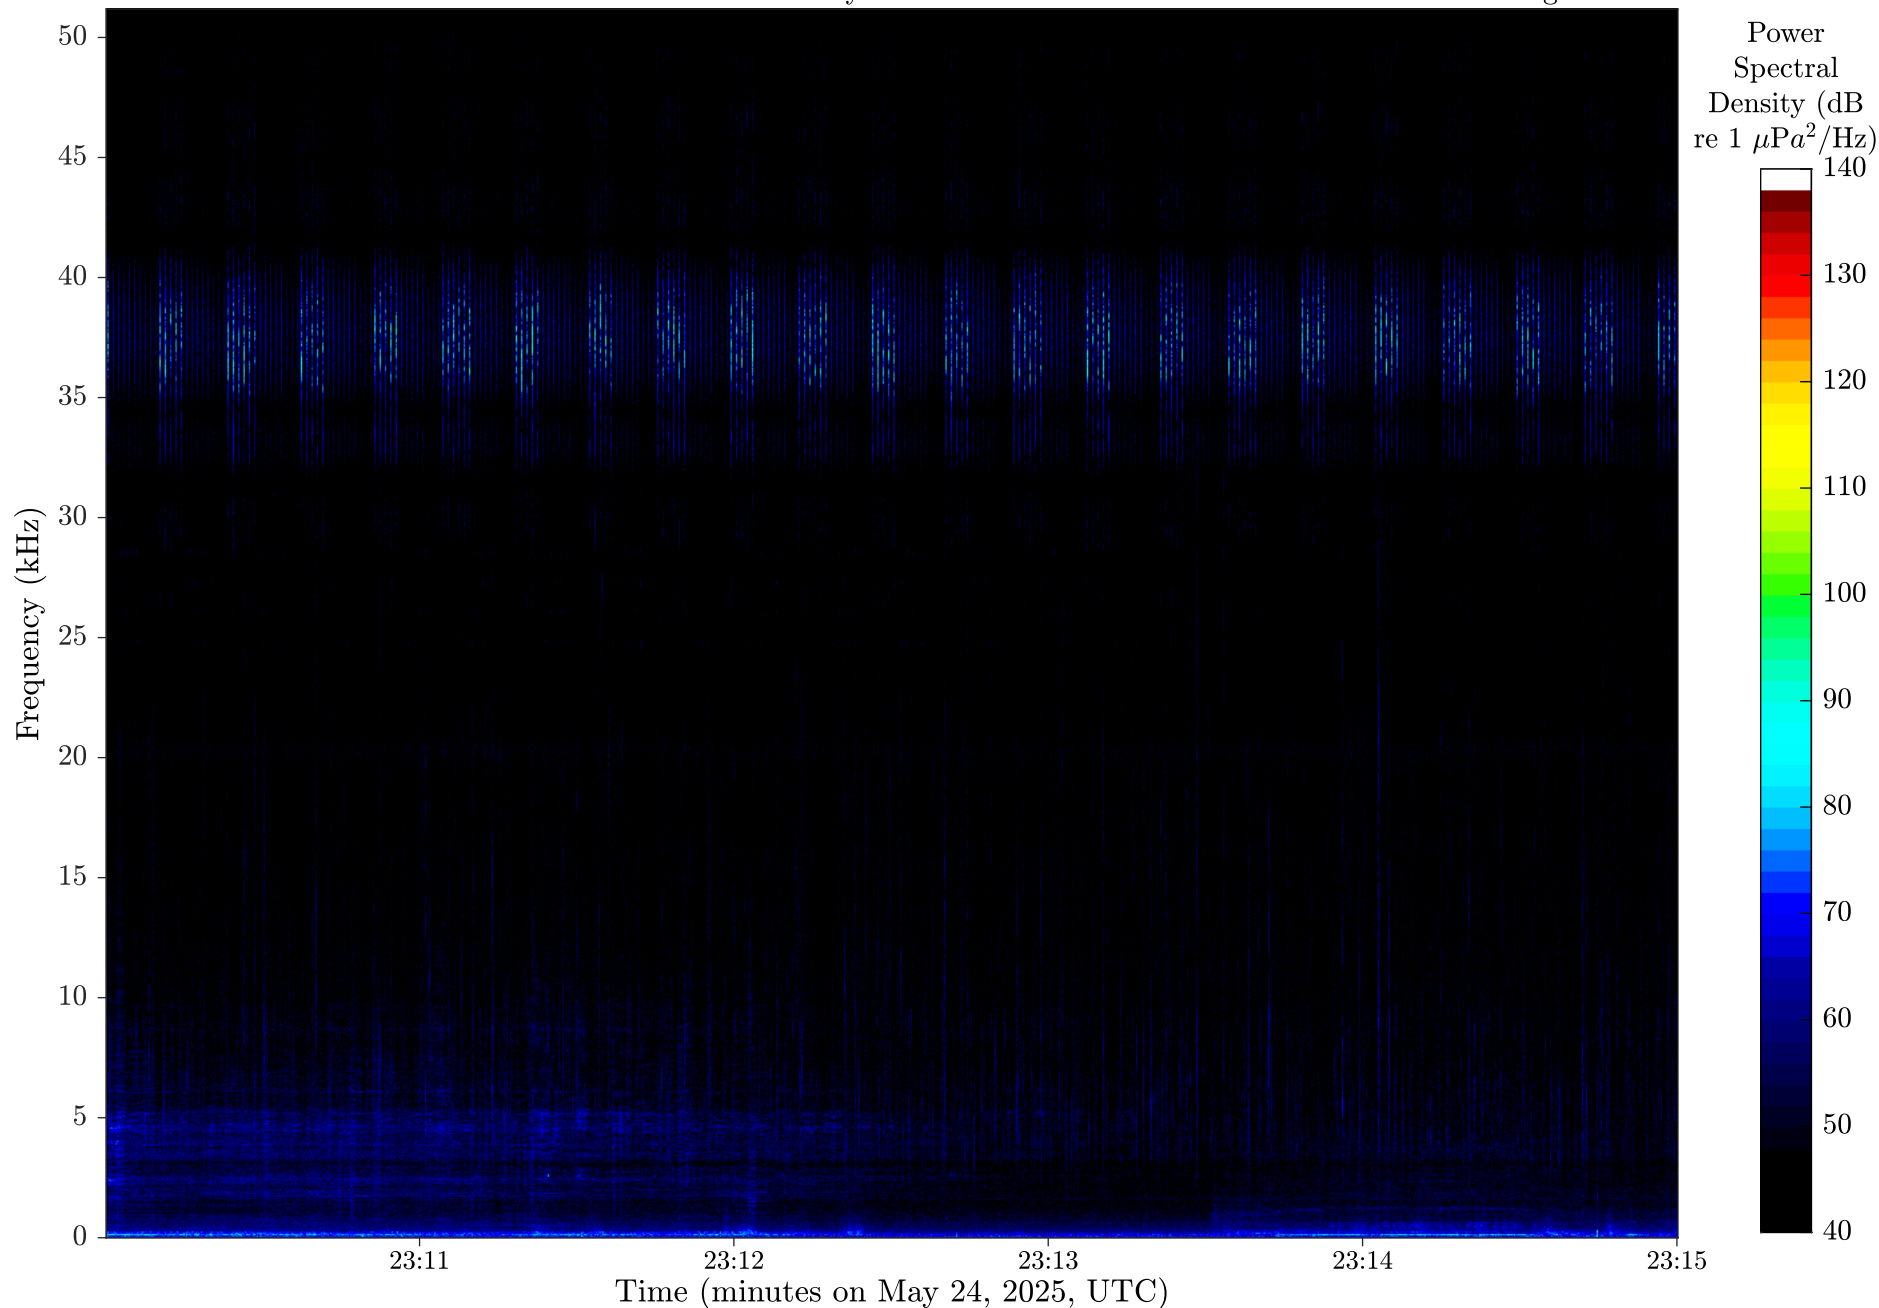


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:59 UTC

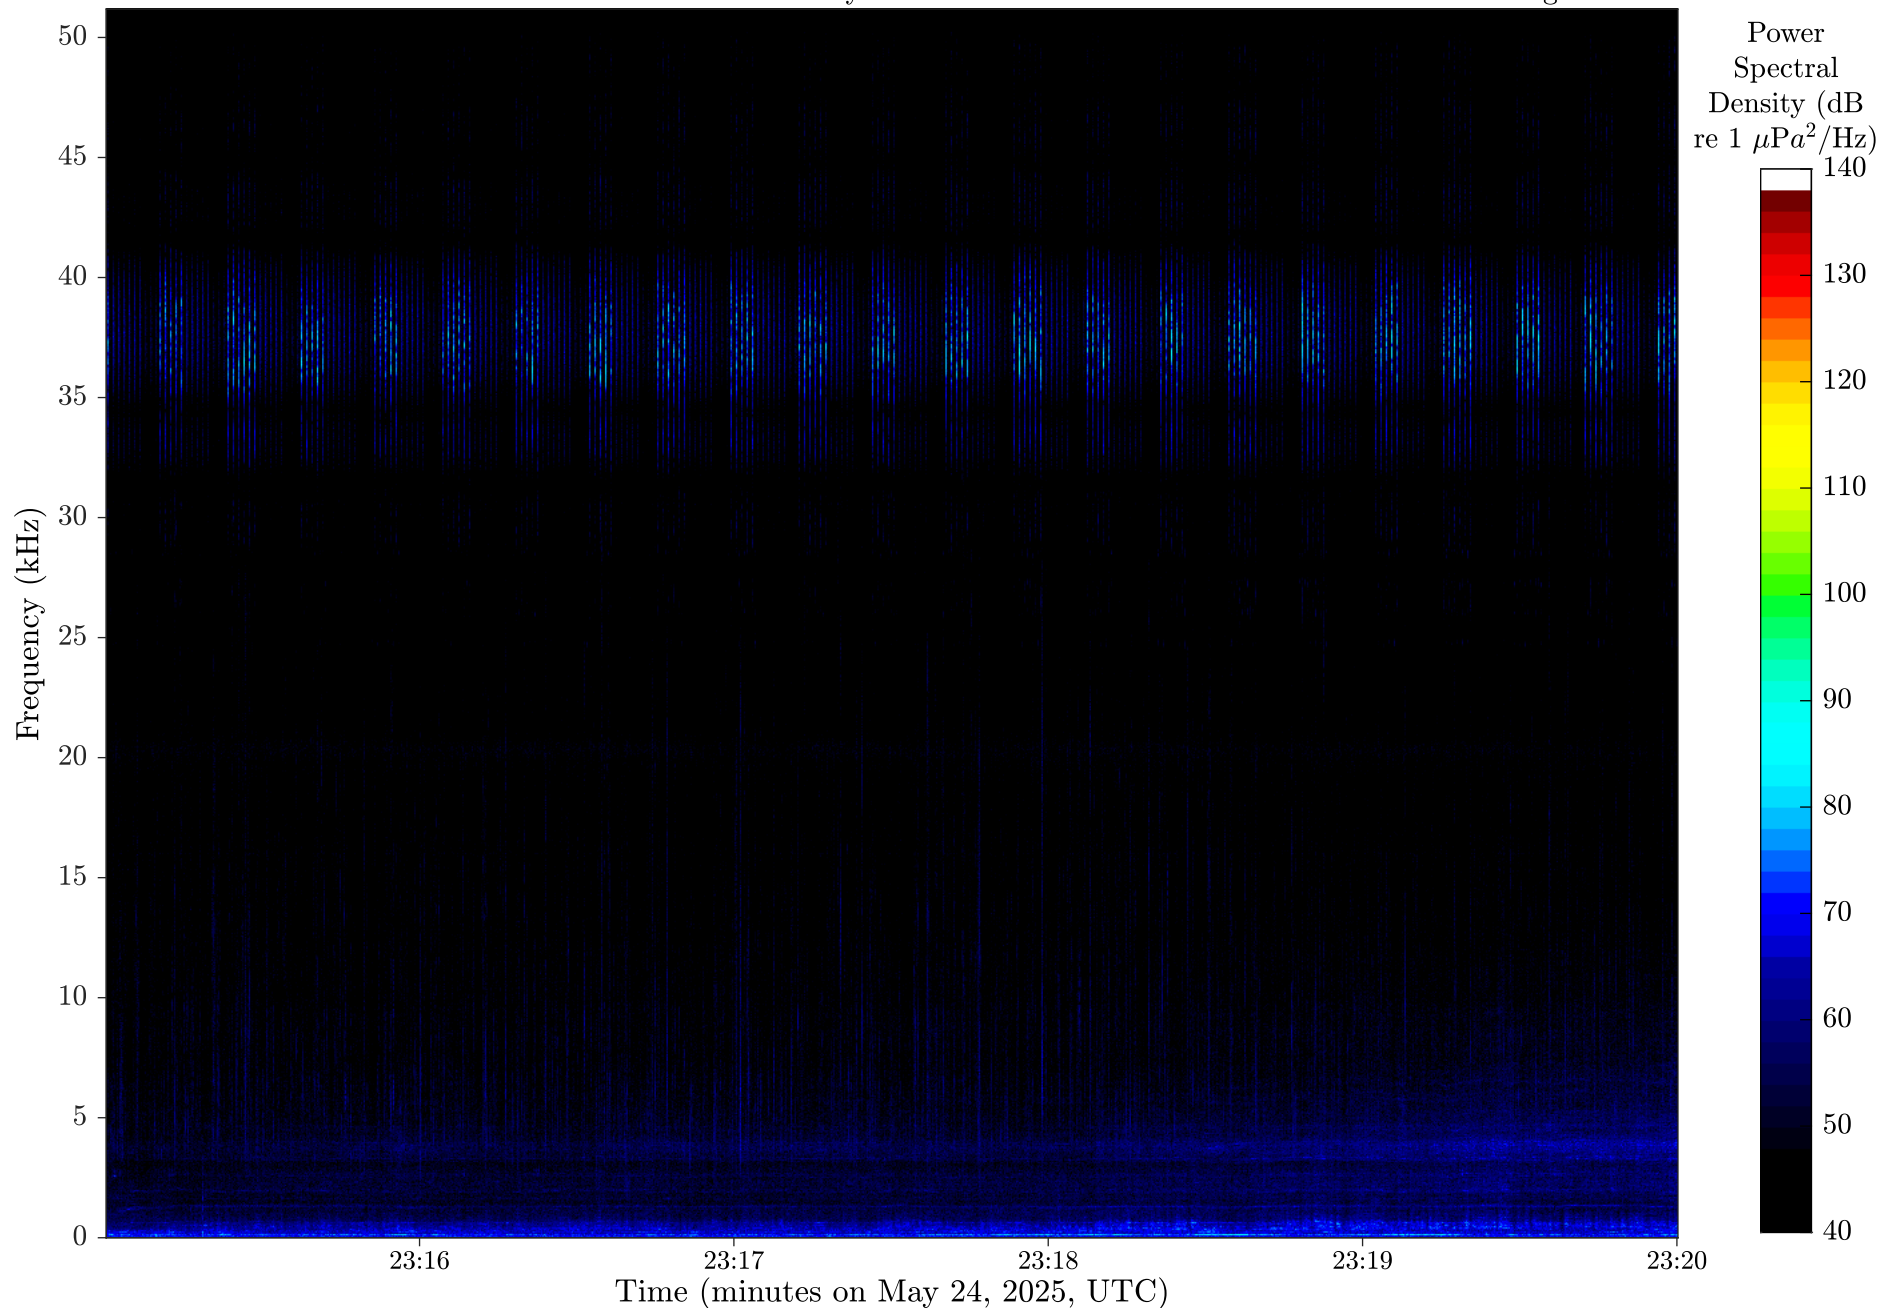


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:45:07 UTC

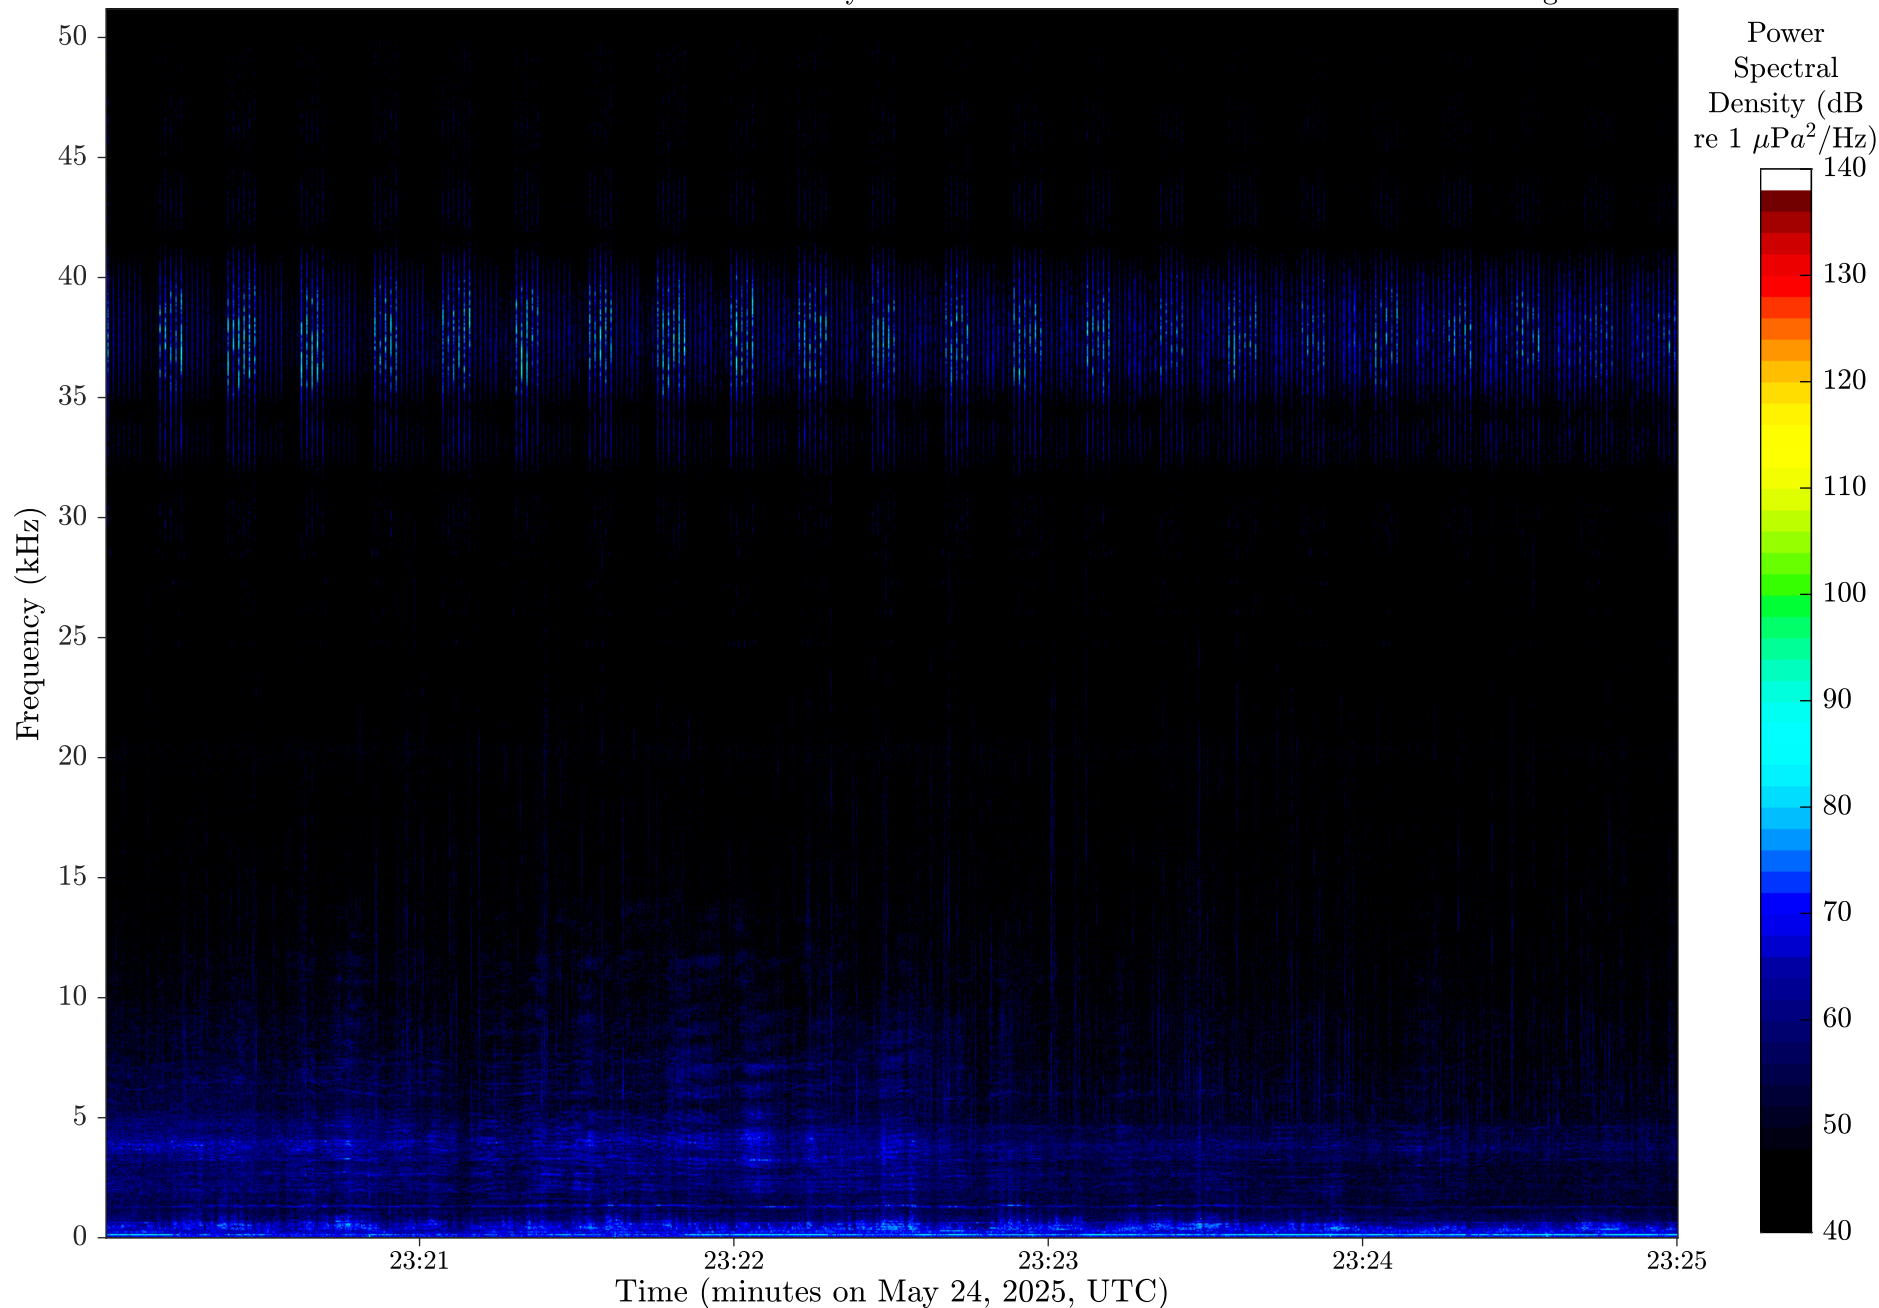


Comments: 30.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:45:14 UTC

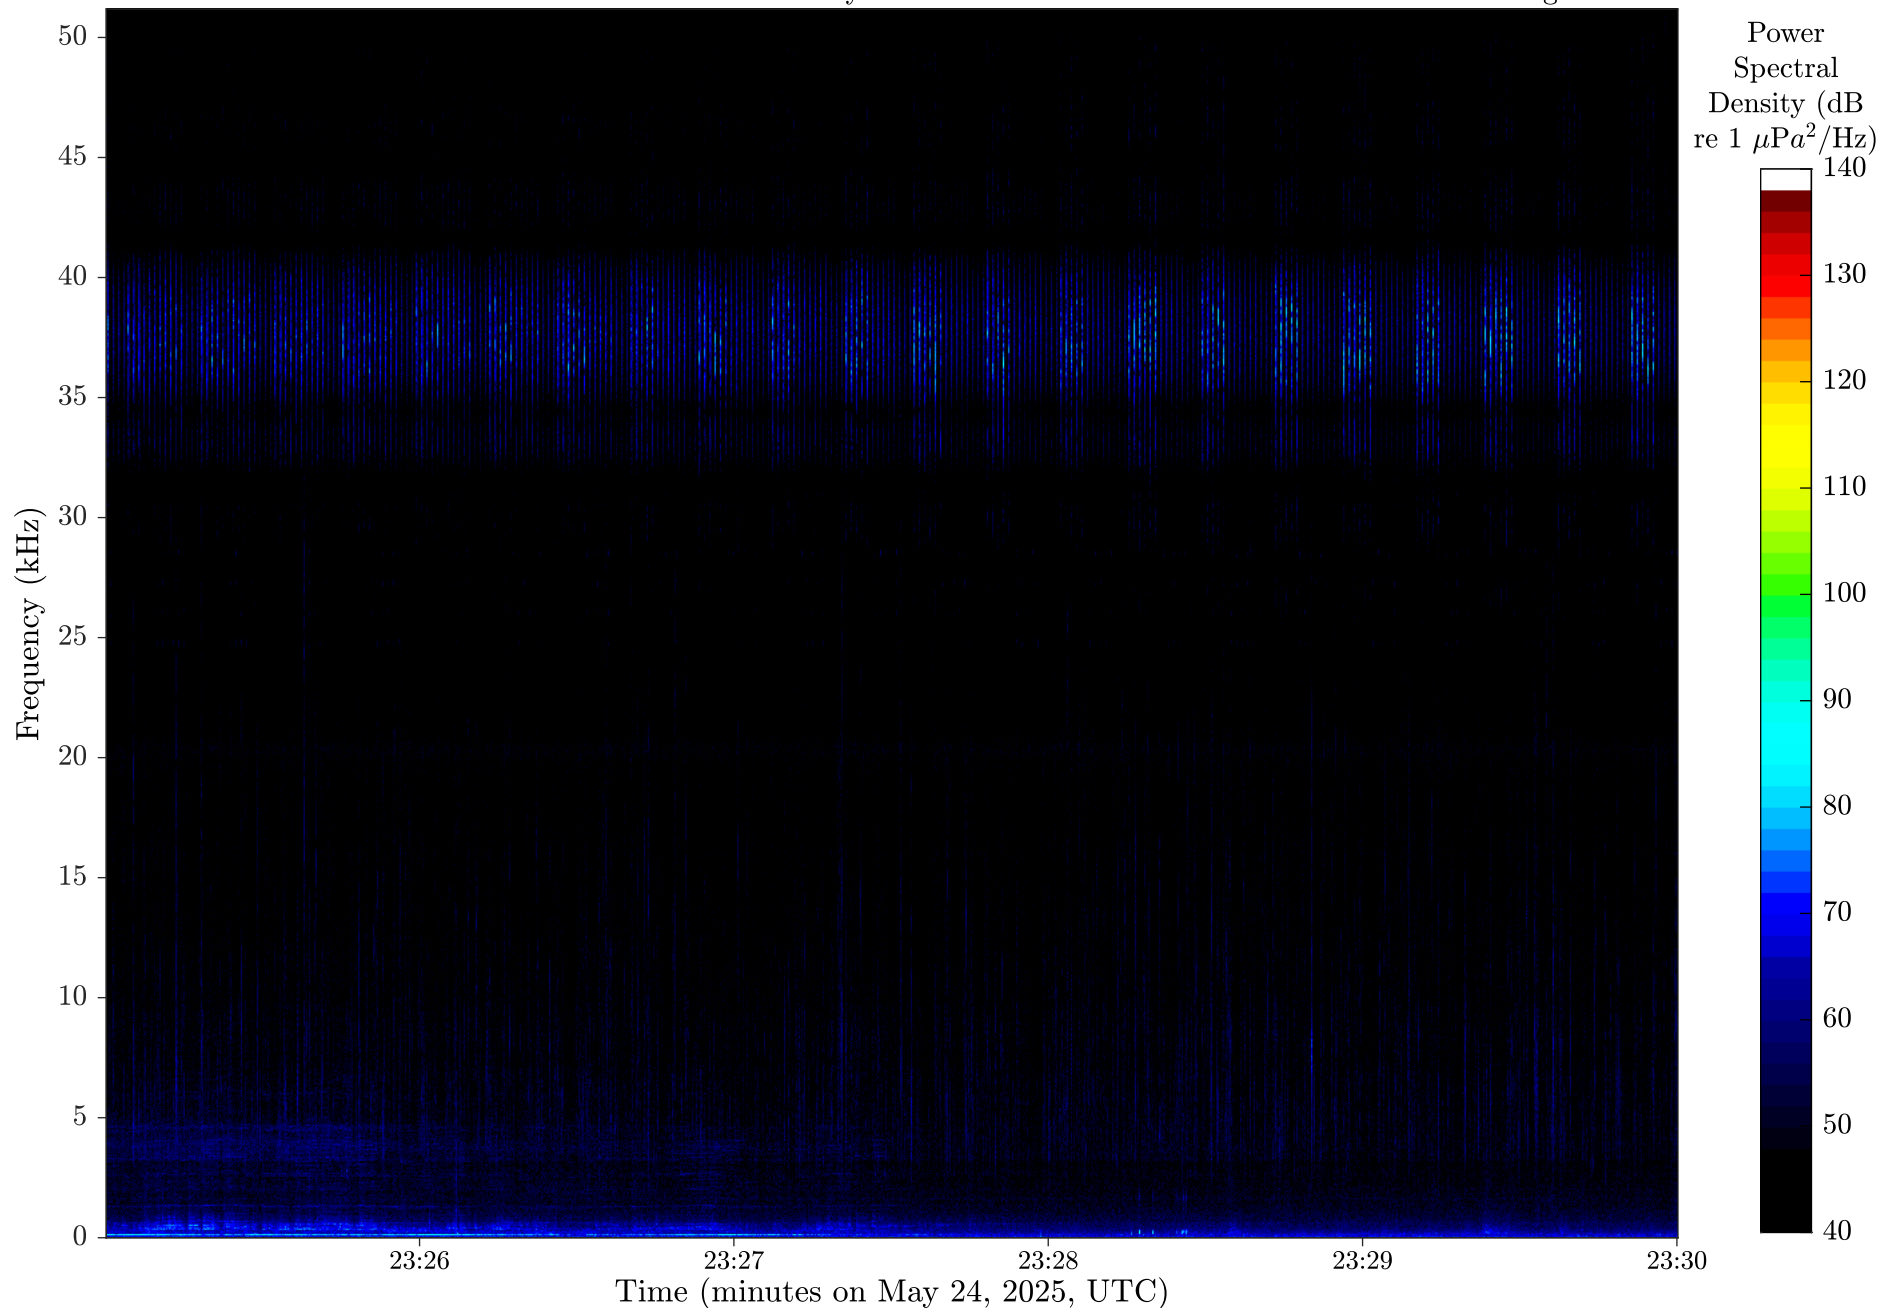


Comments: 31.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:45:22 UTC

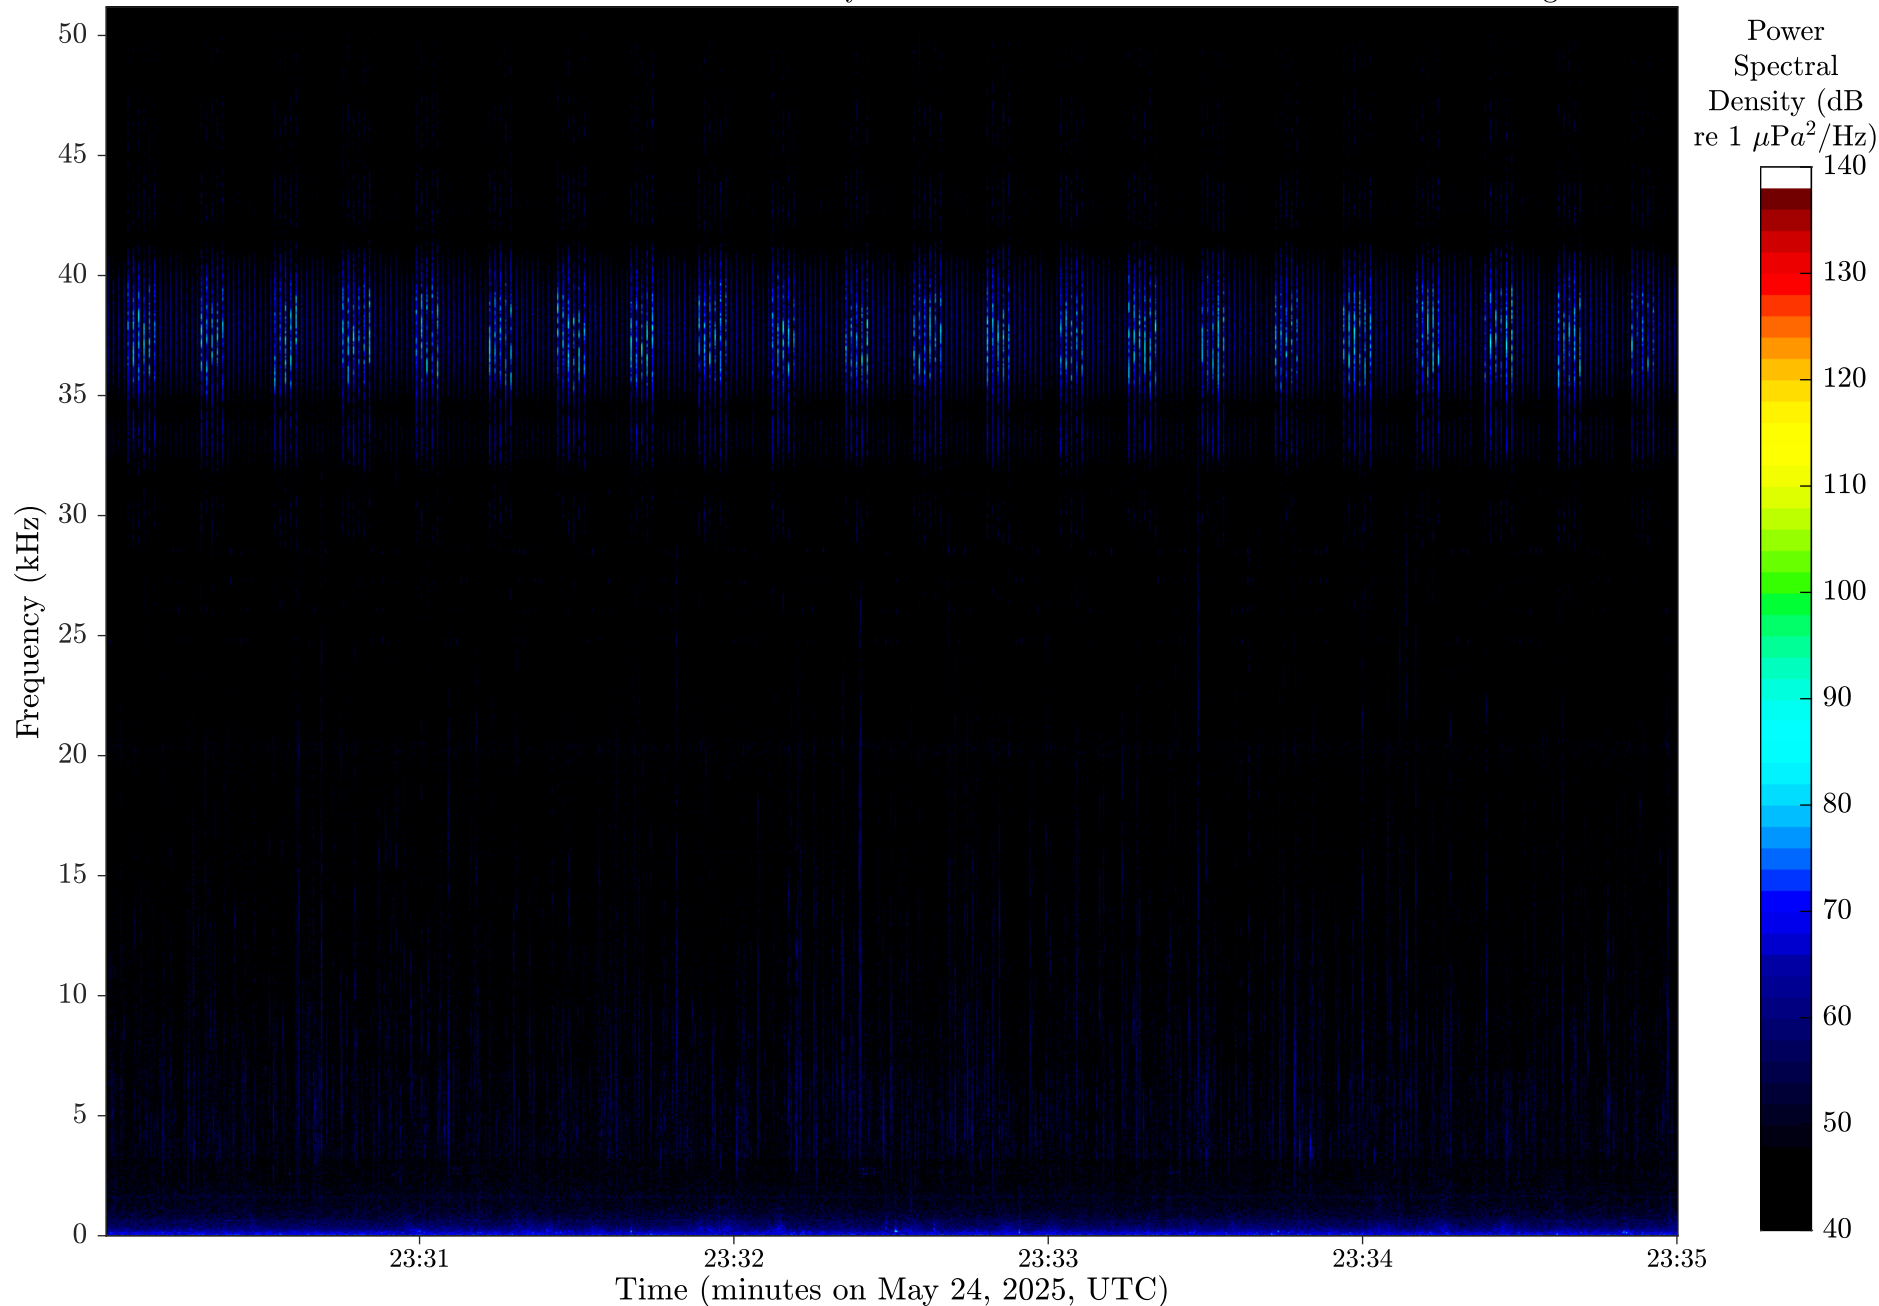

Comments: 33.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:45:29 UTC

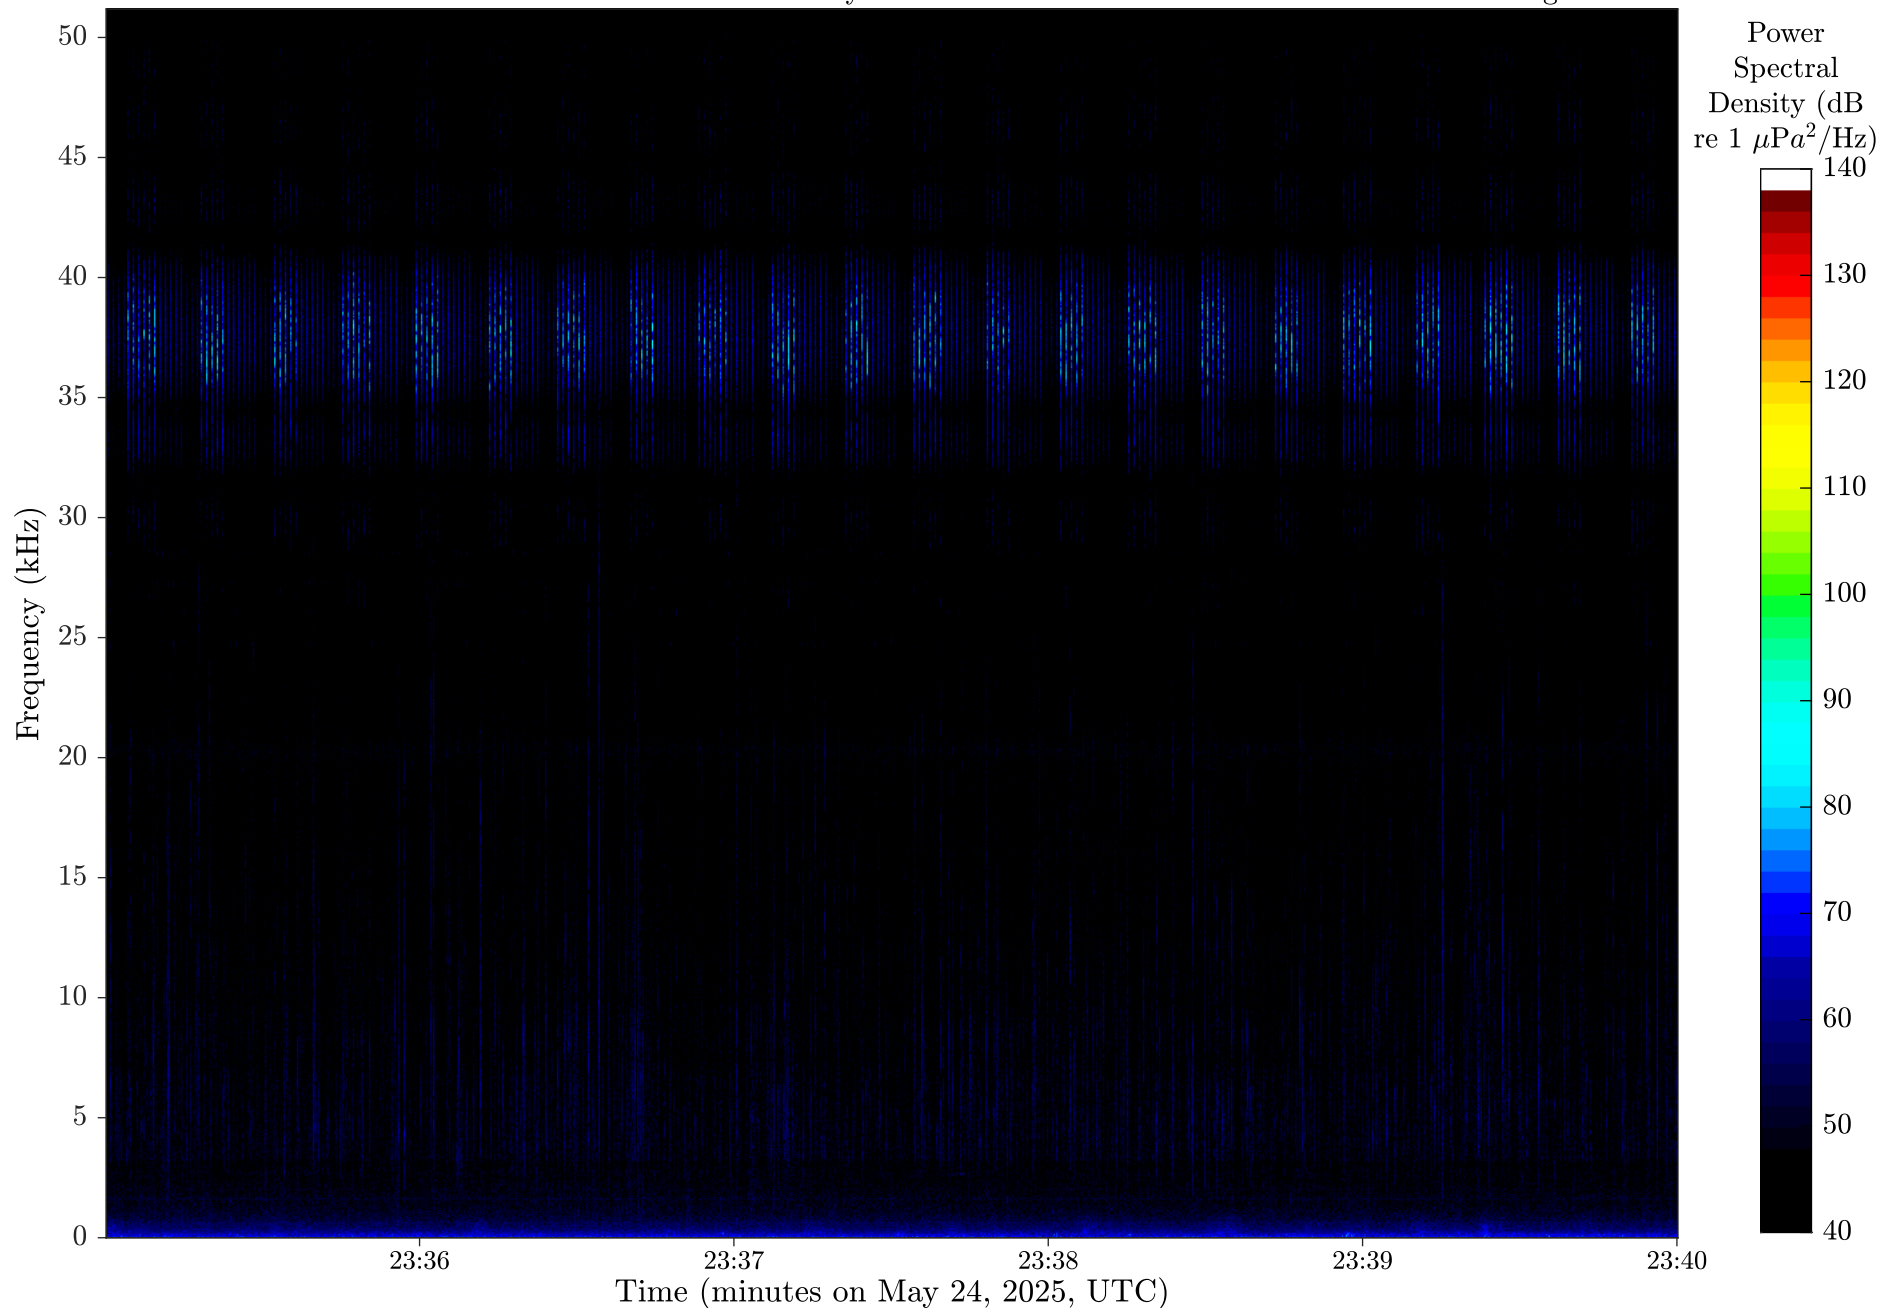


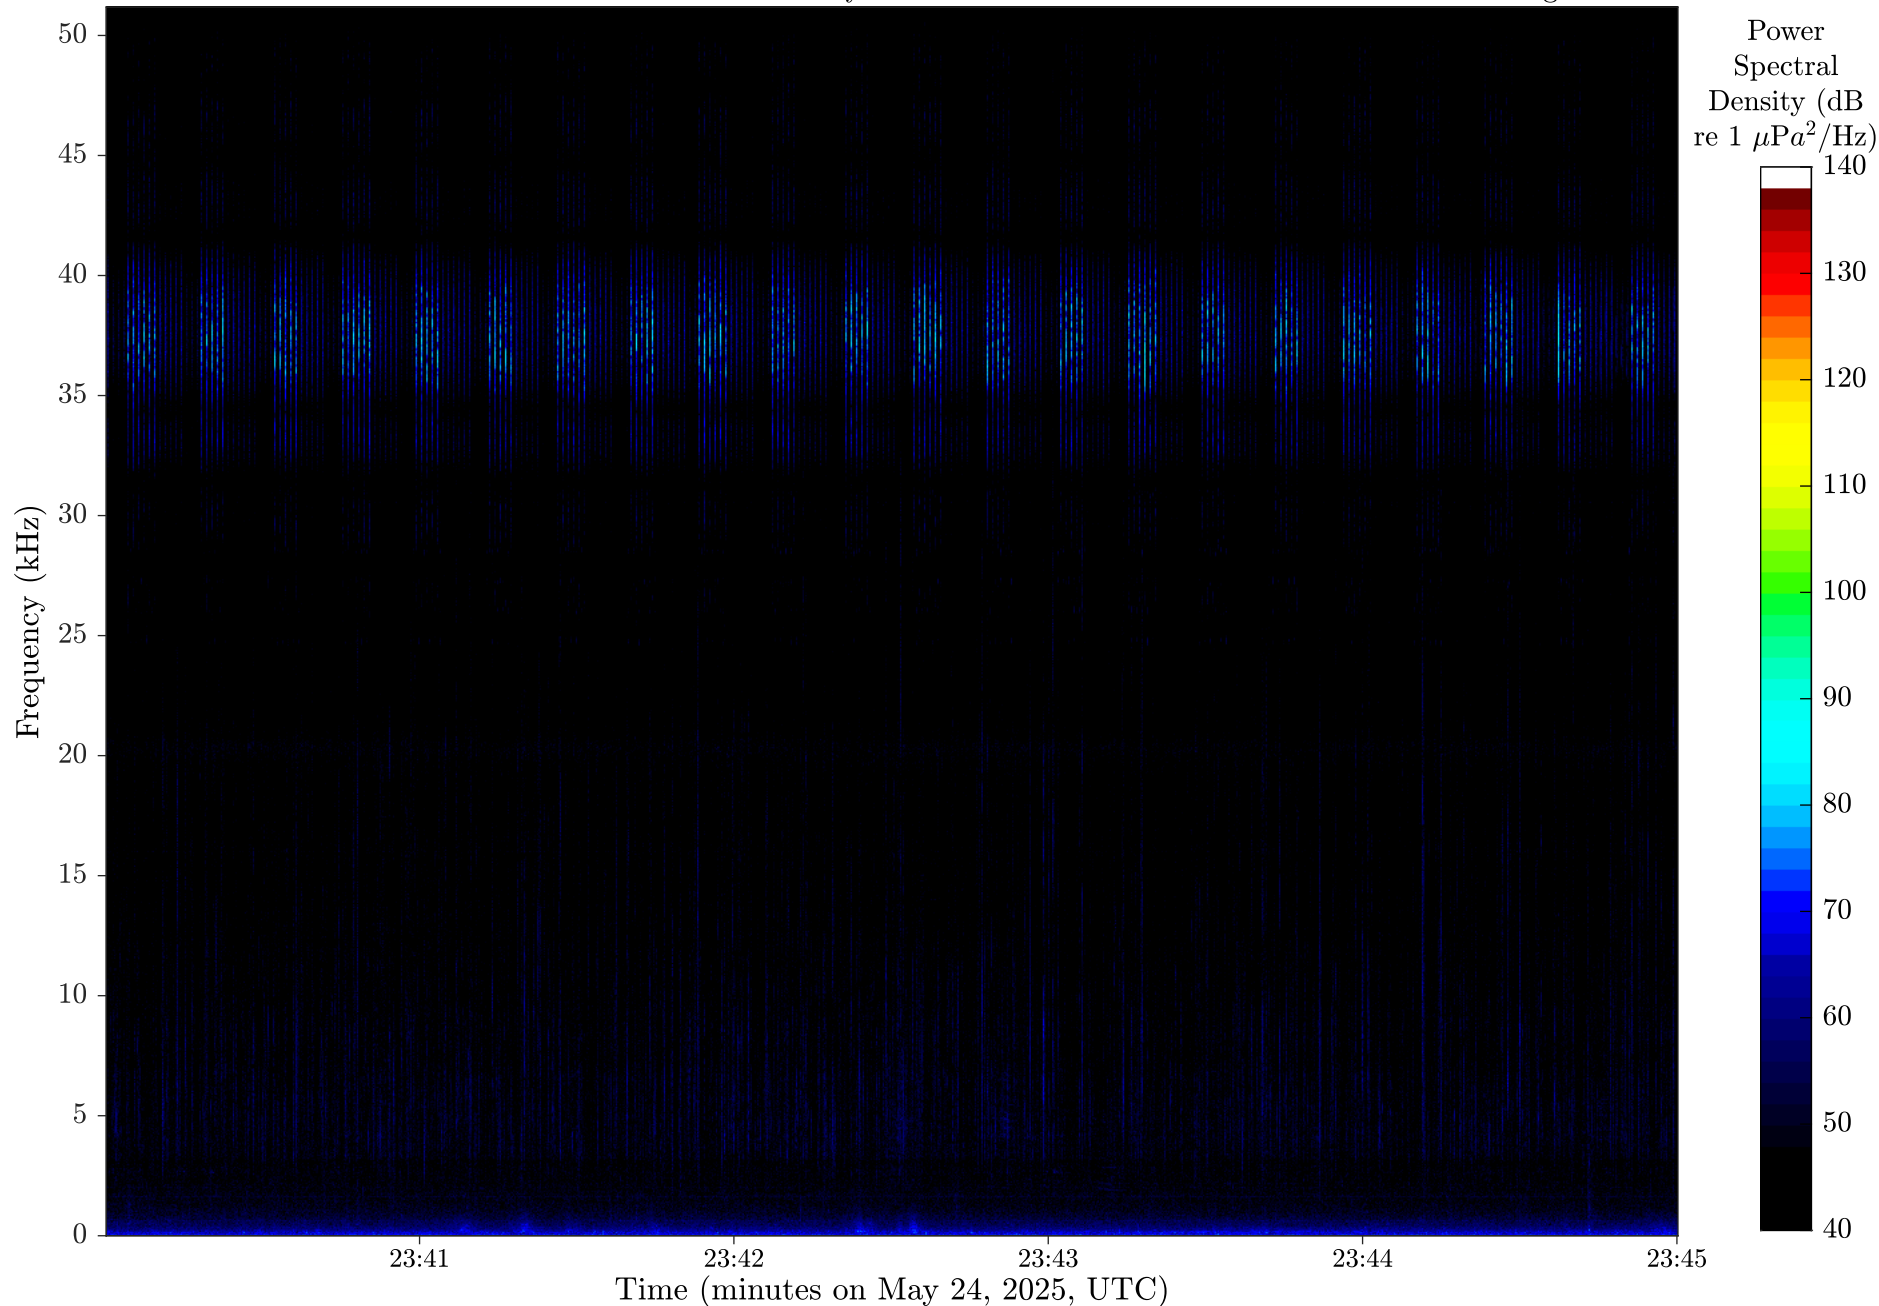

Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:45:45 UTC

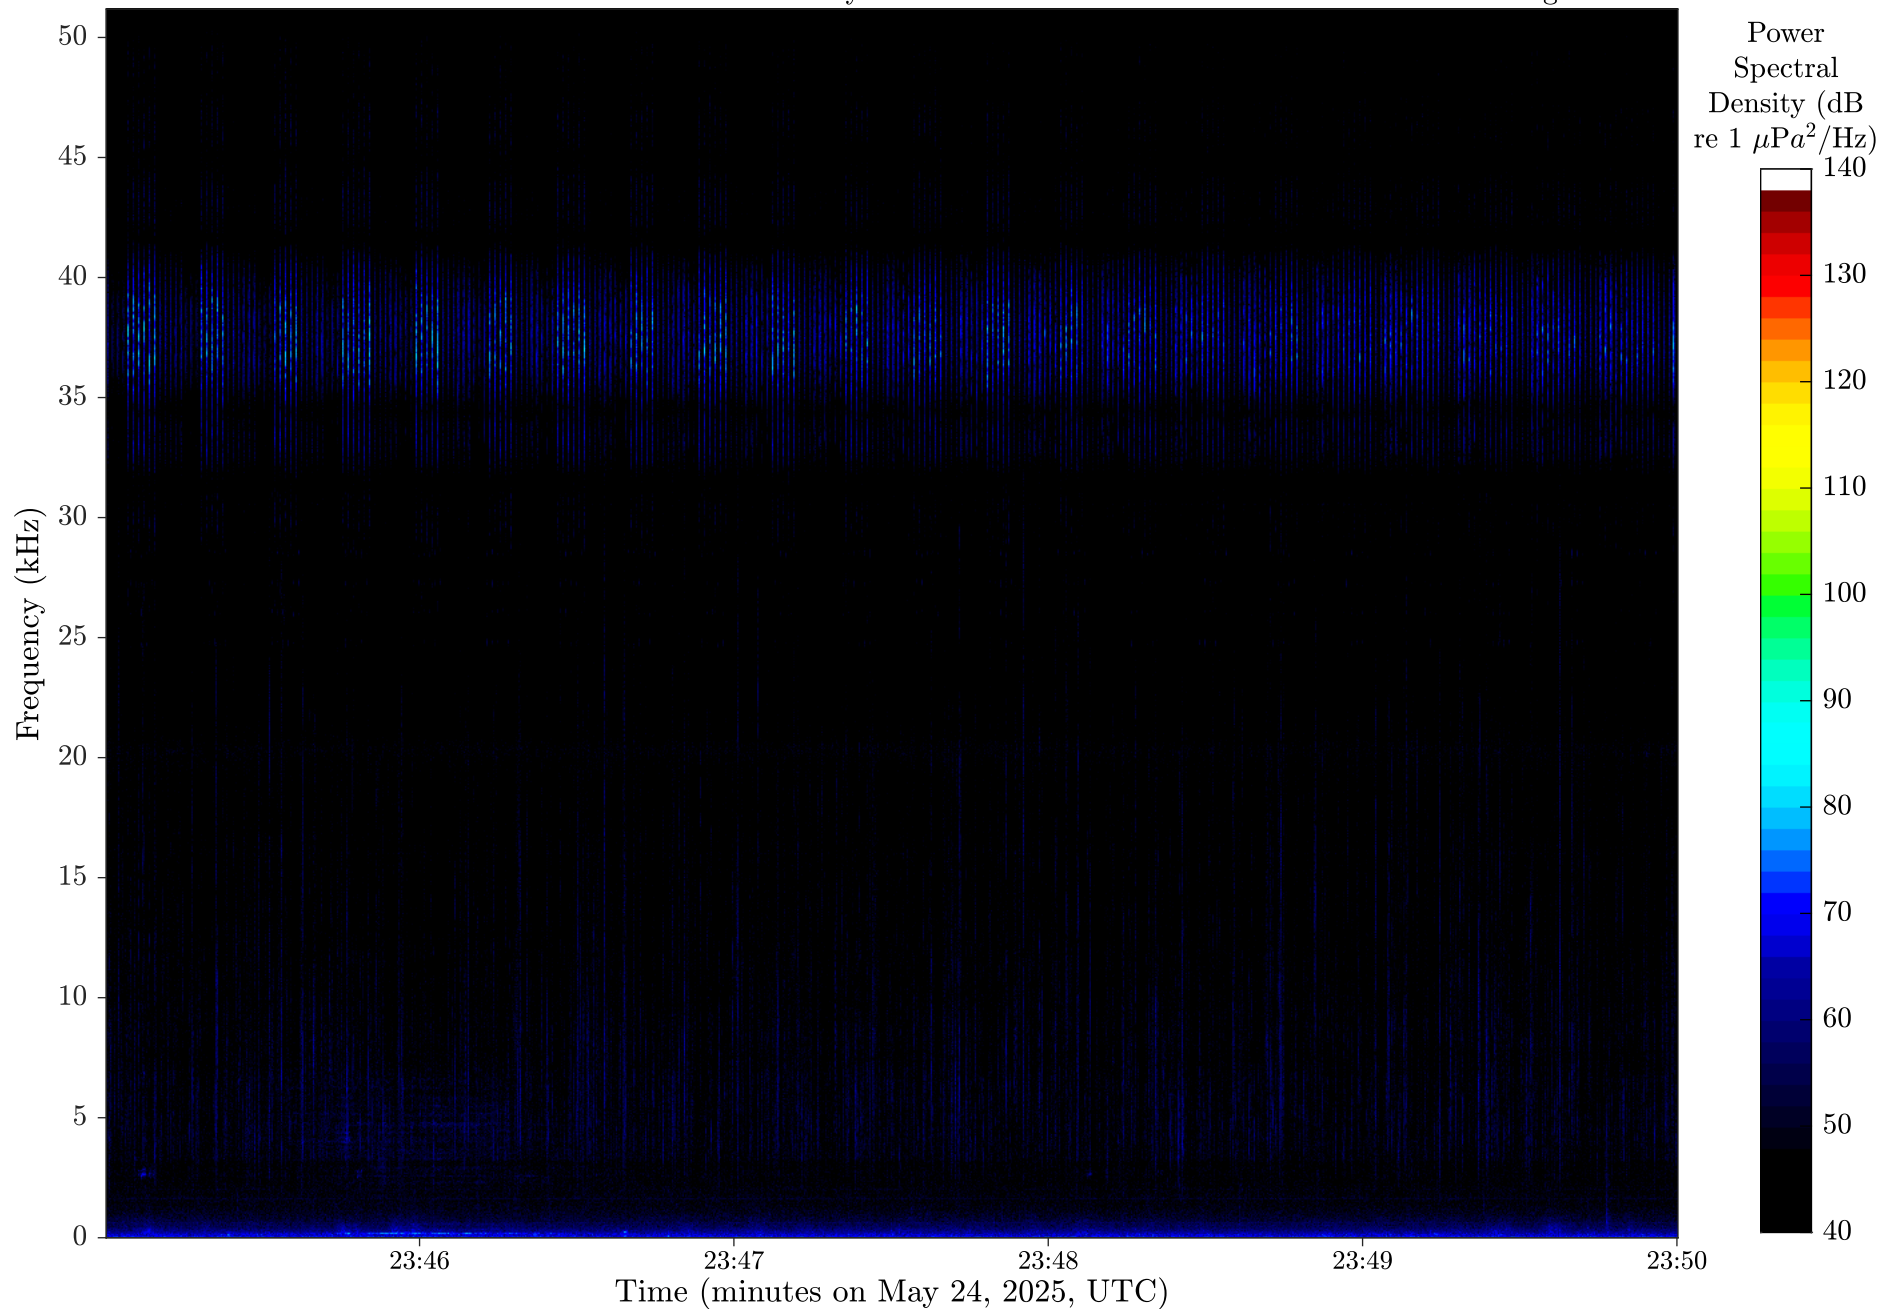

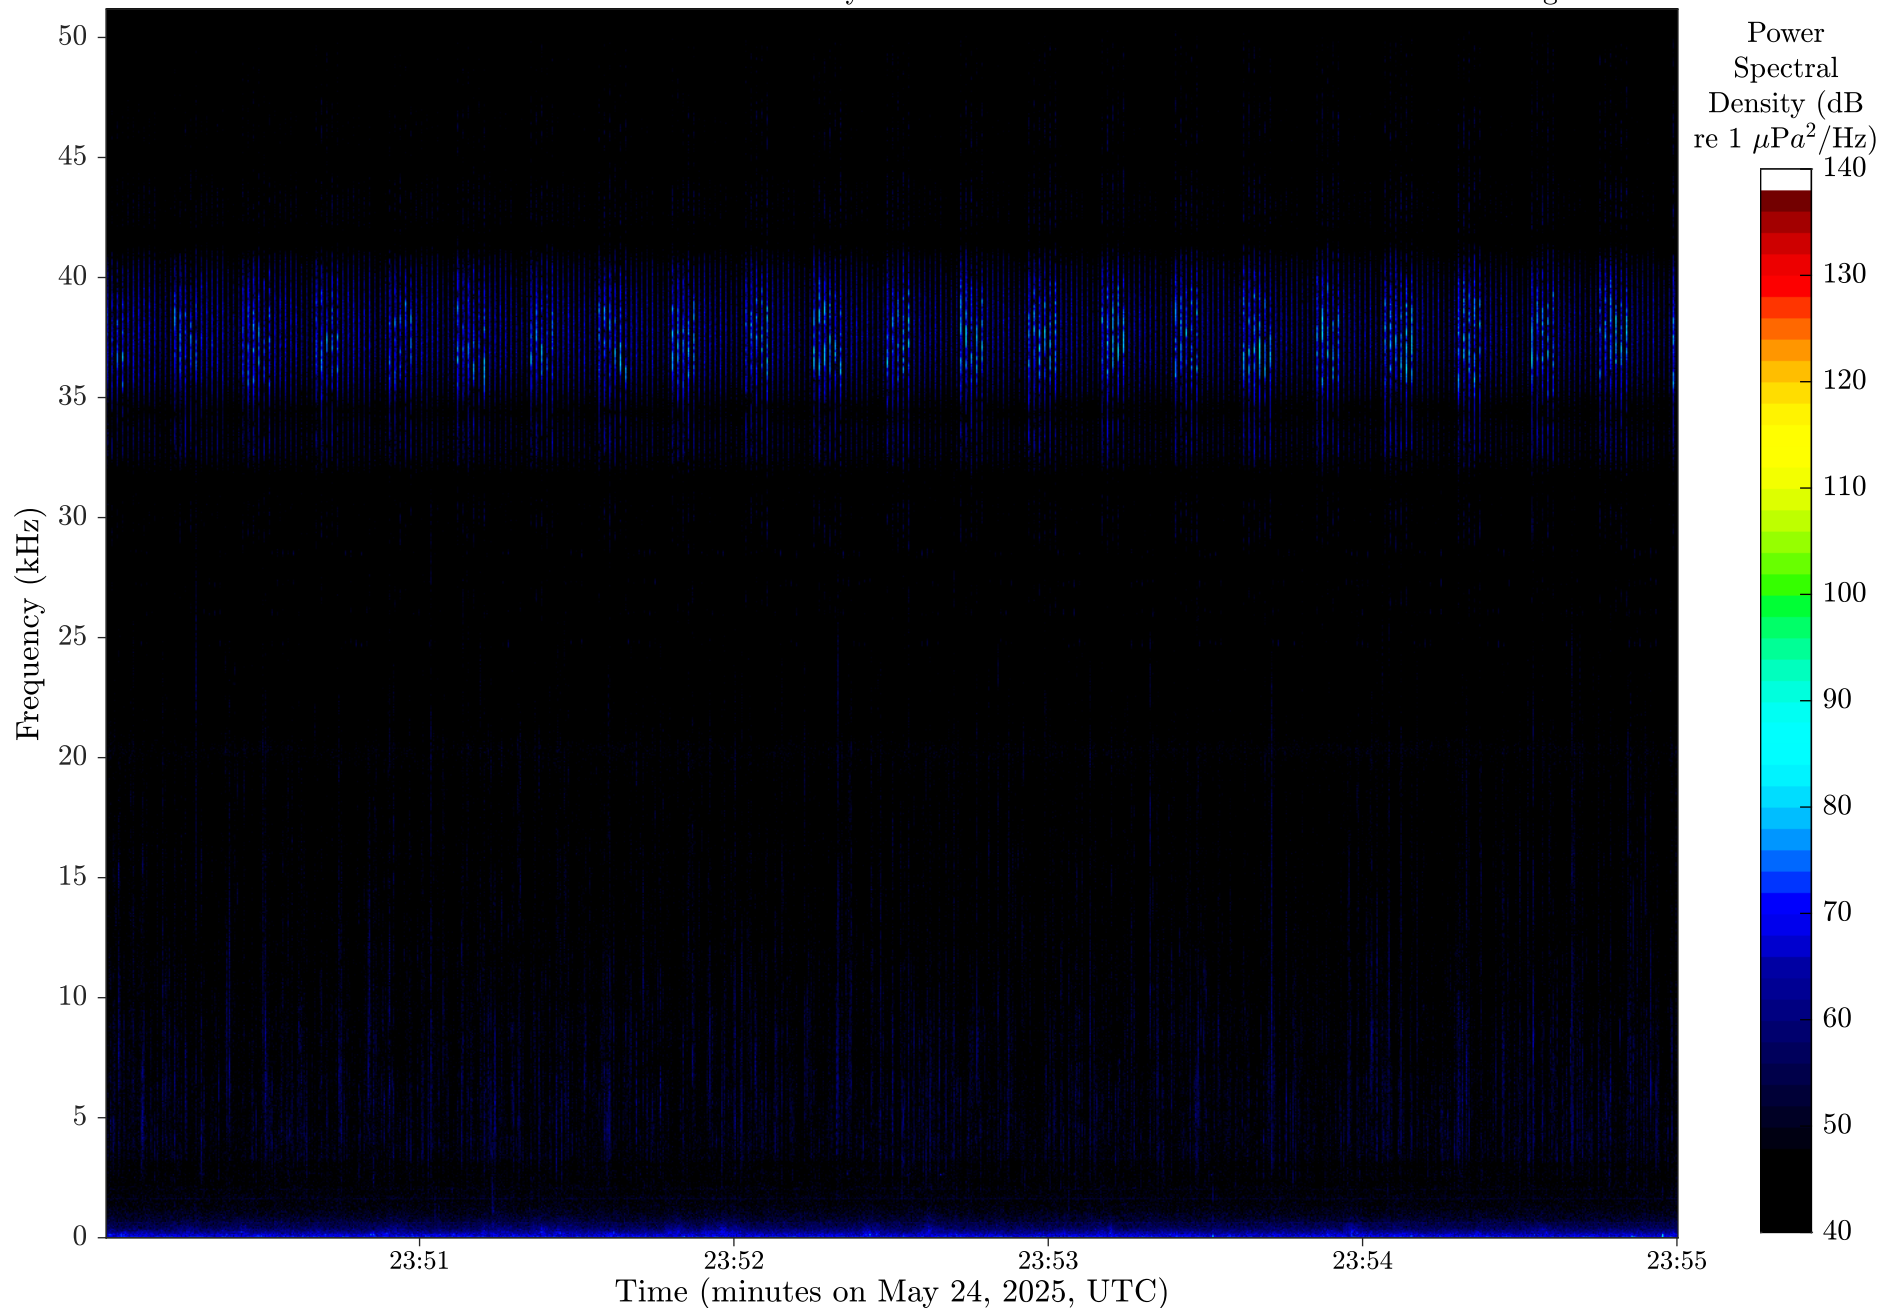

Comments: 34.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:00 UTC

