



Comments: 31.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:12:15 UTC

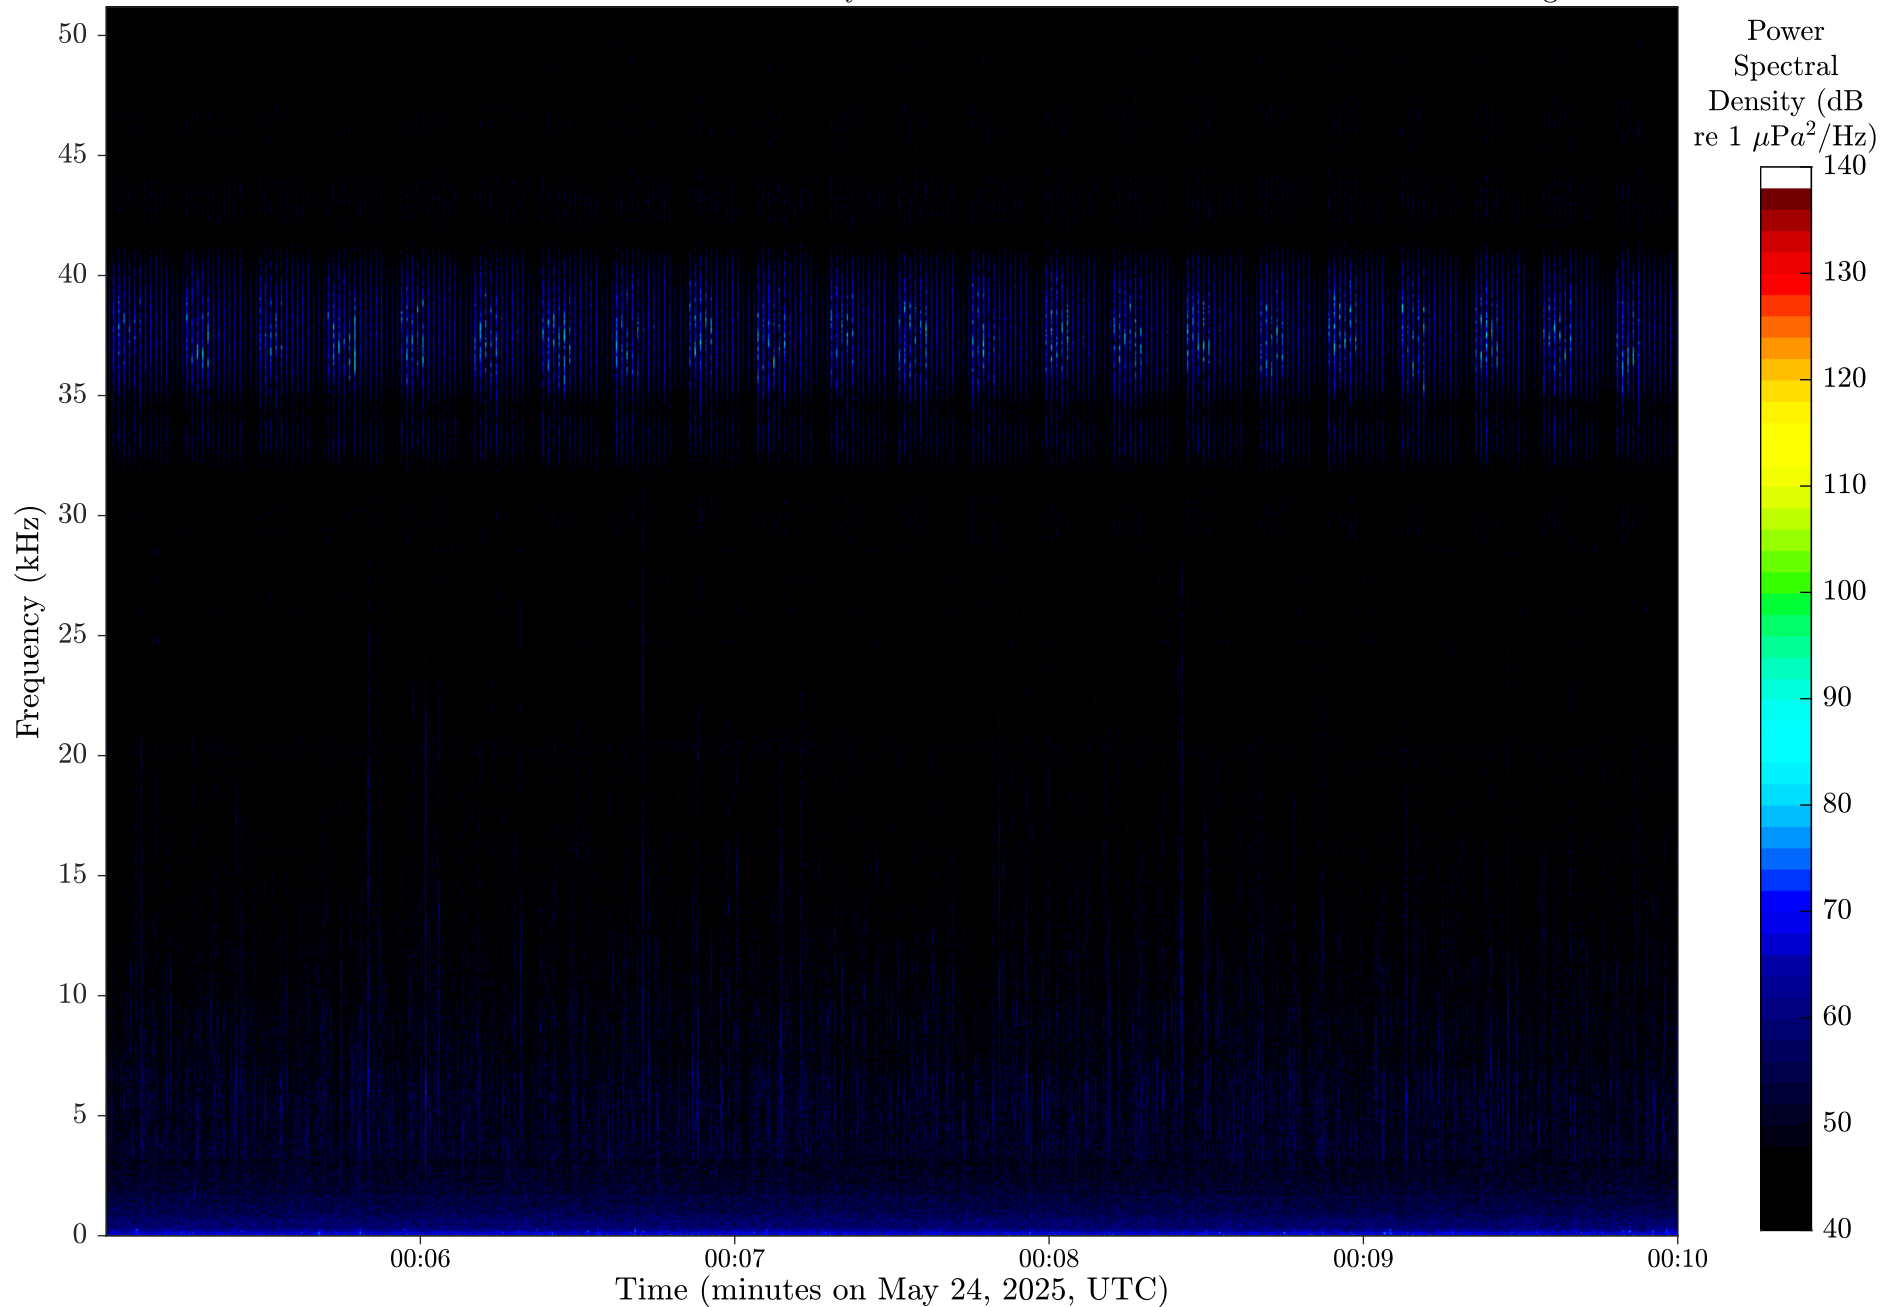


Comments: 32.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:12:23 UTC

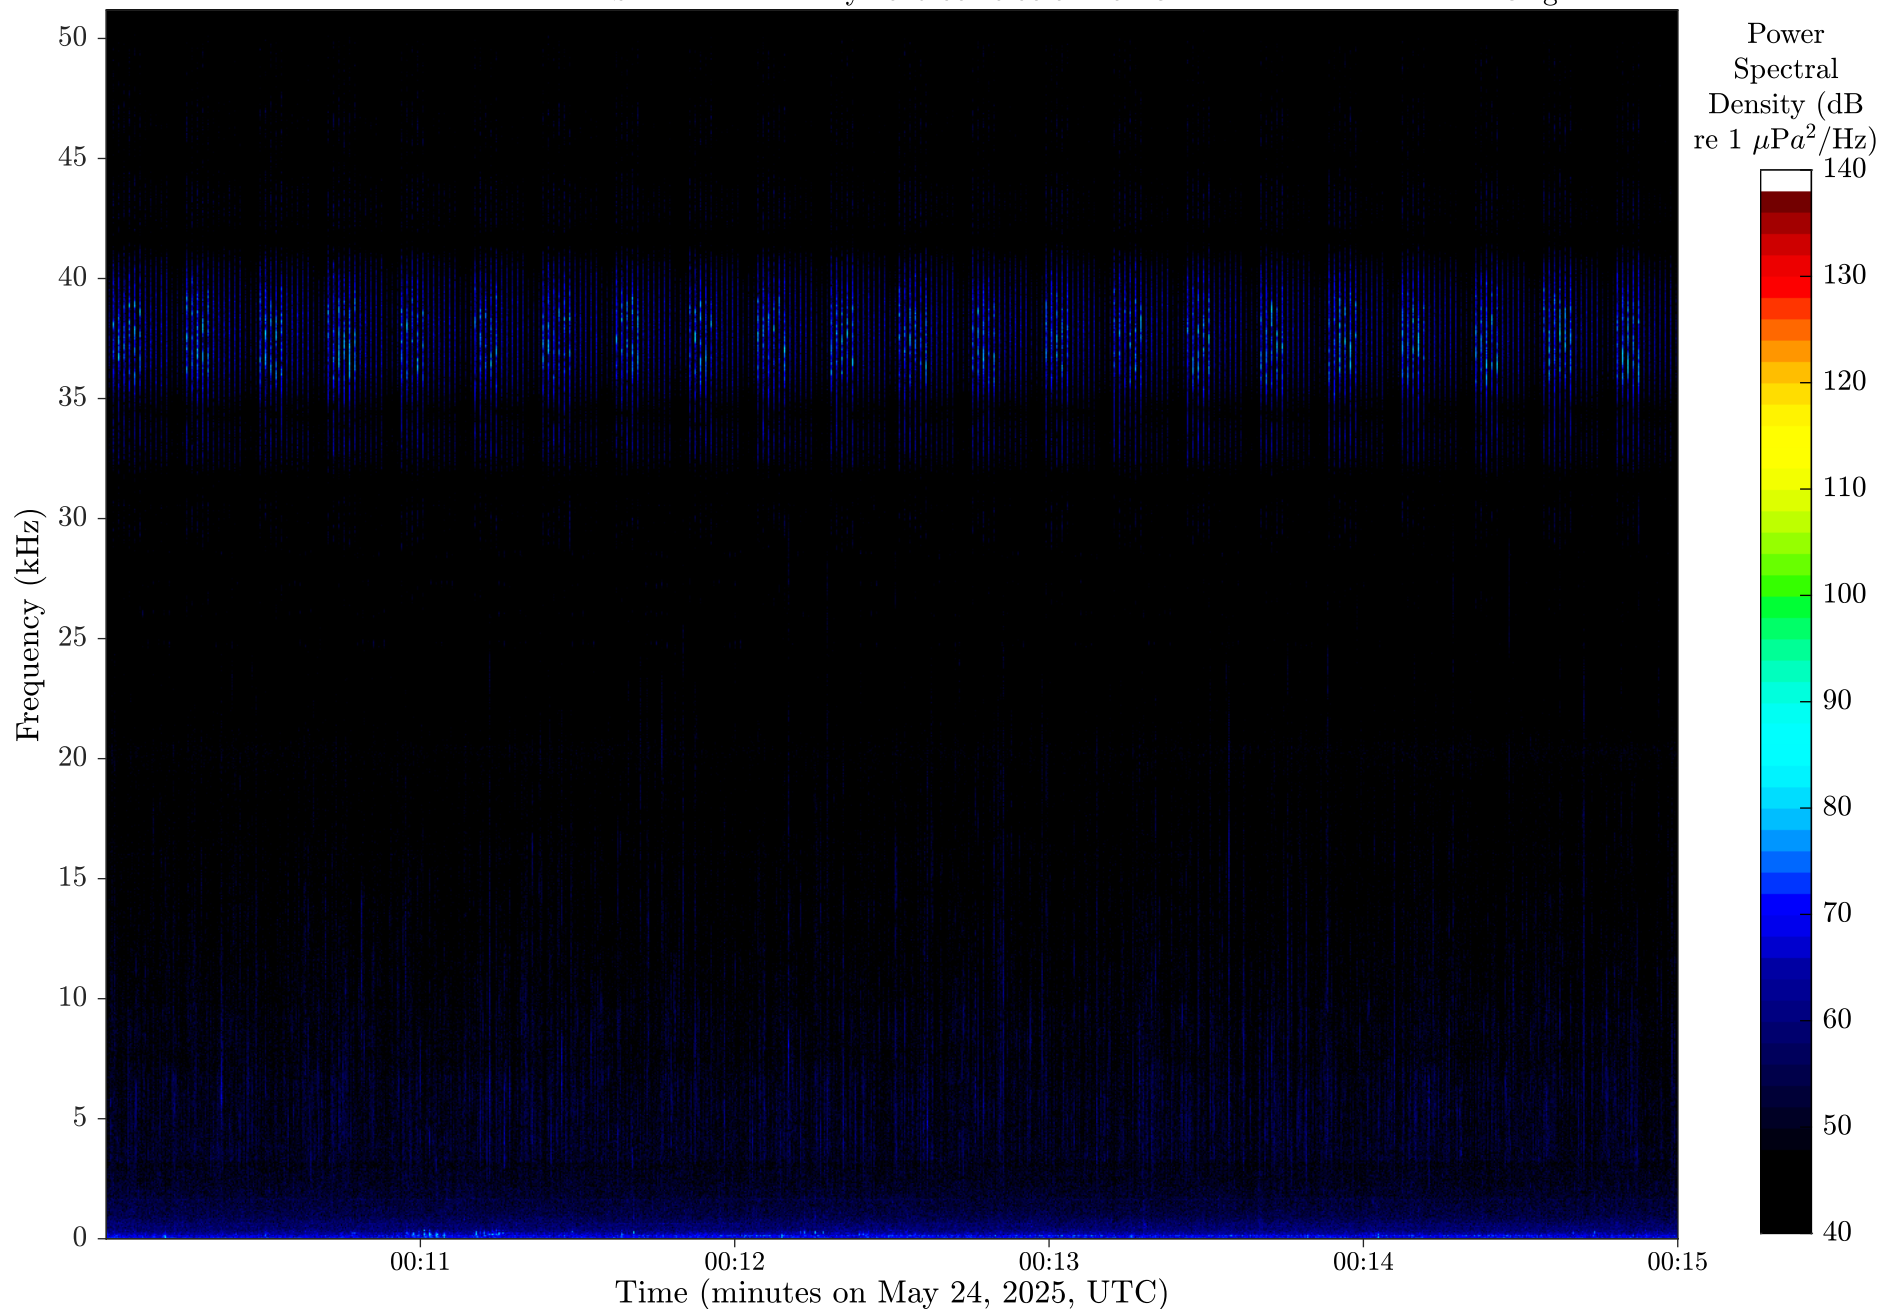


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:12:30 UTC

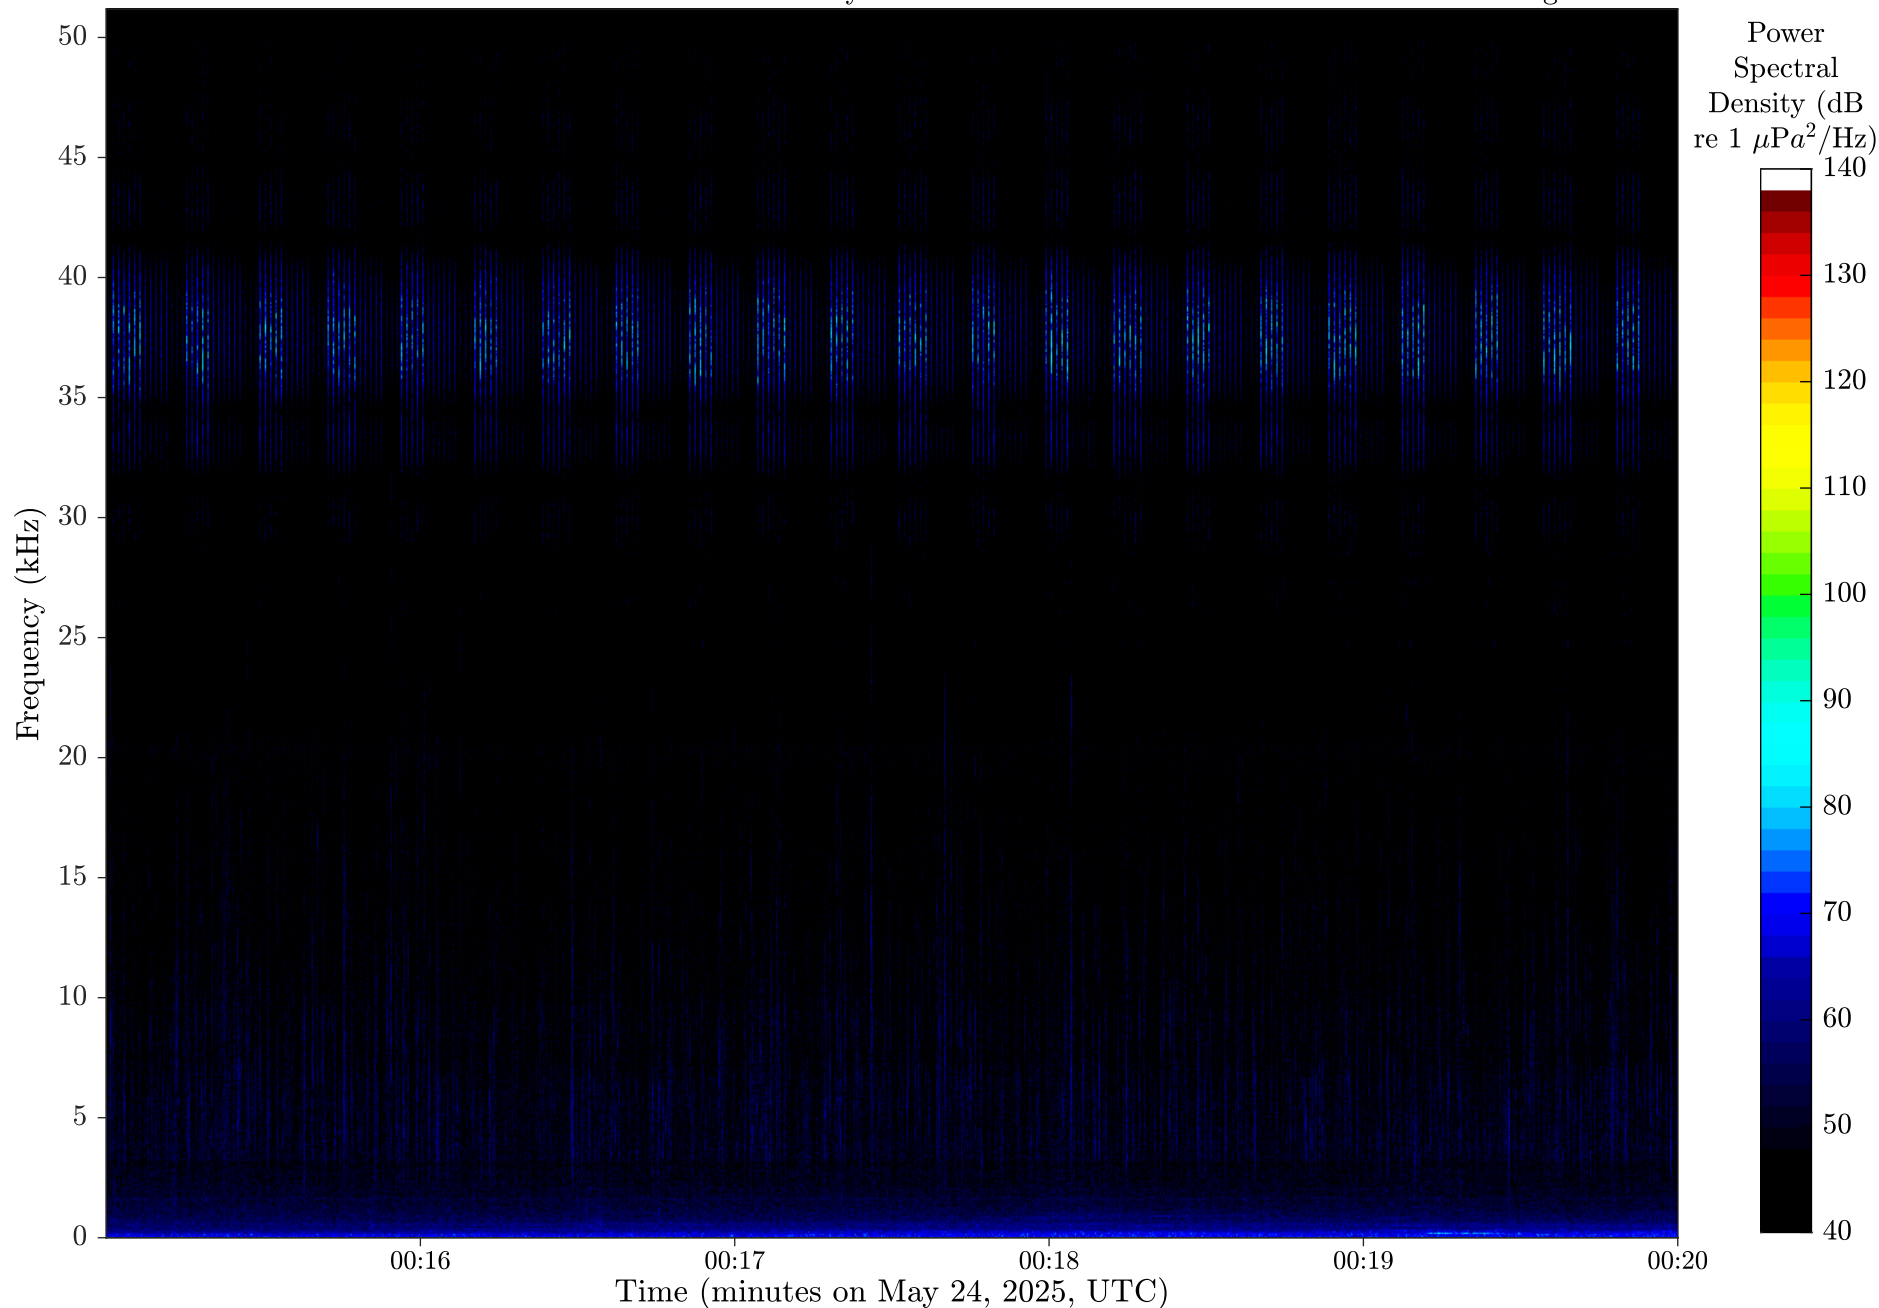


Comments: 35.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:12:38 UTC

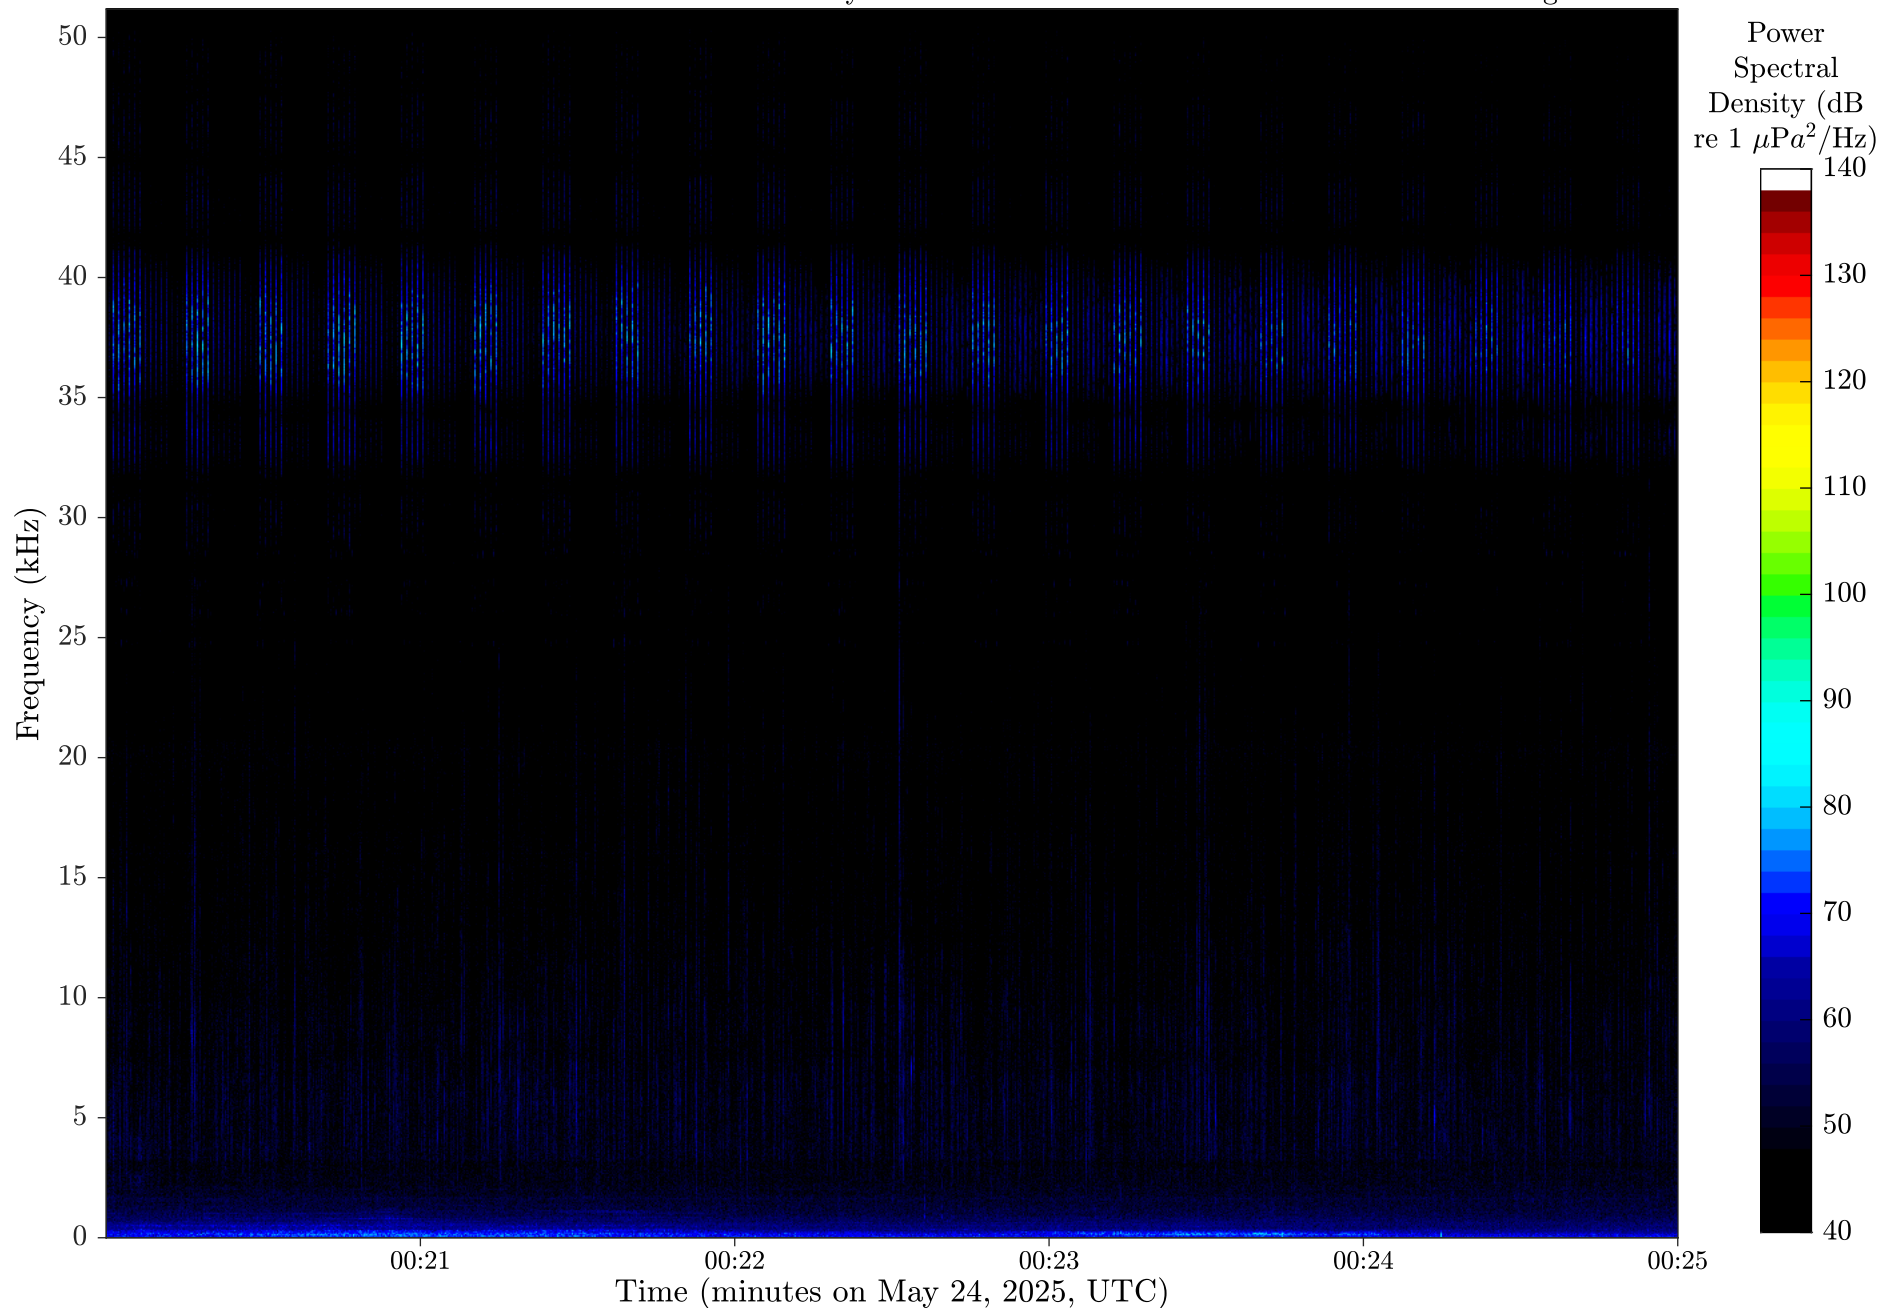

Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:12:45 UTC

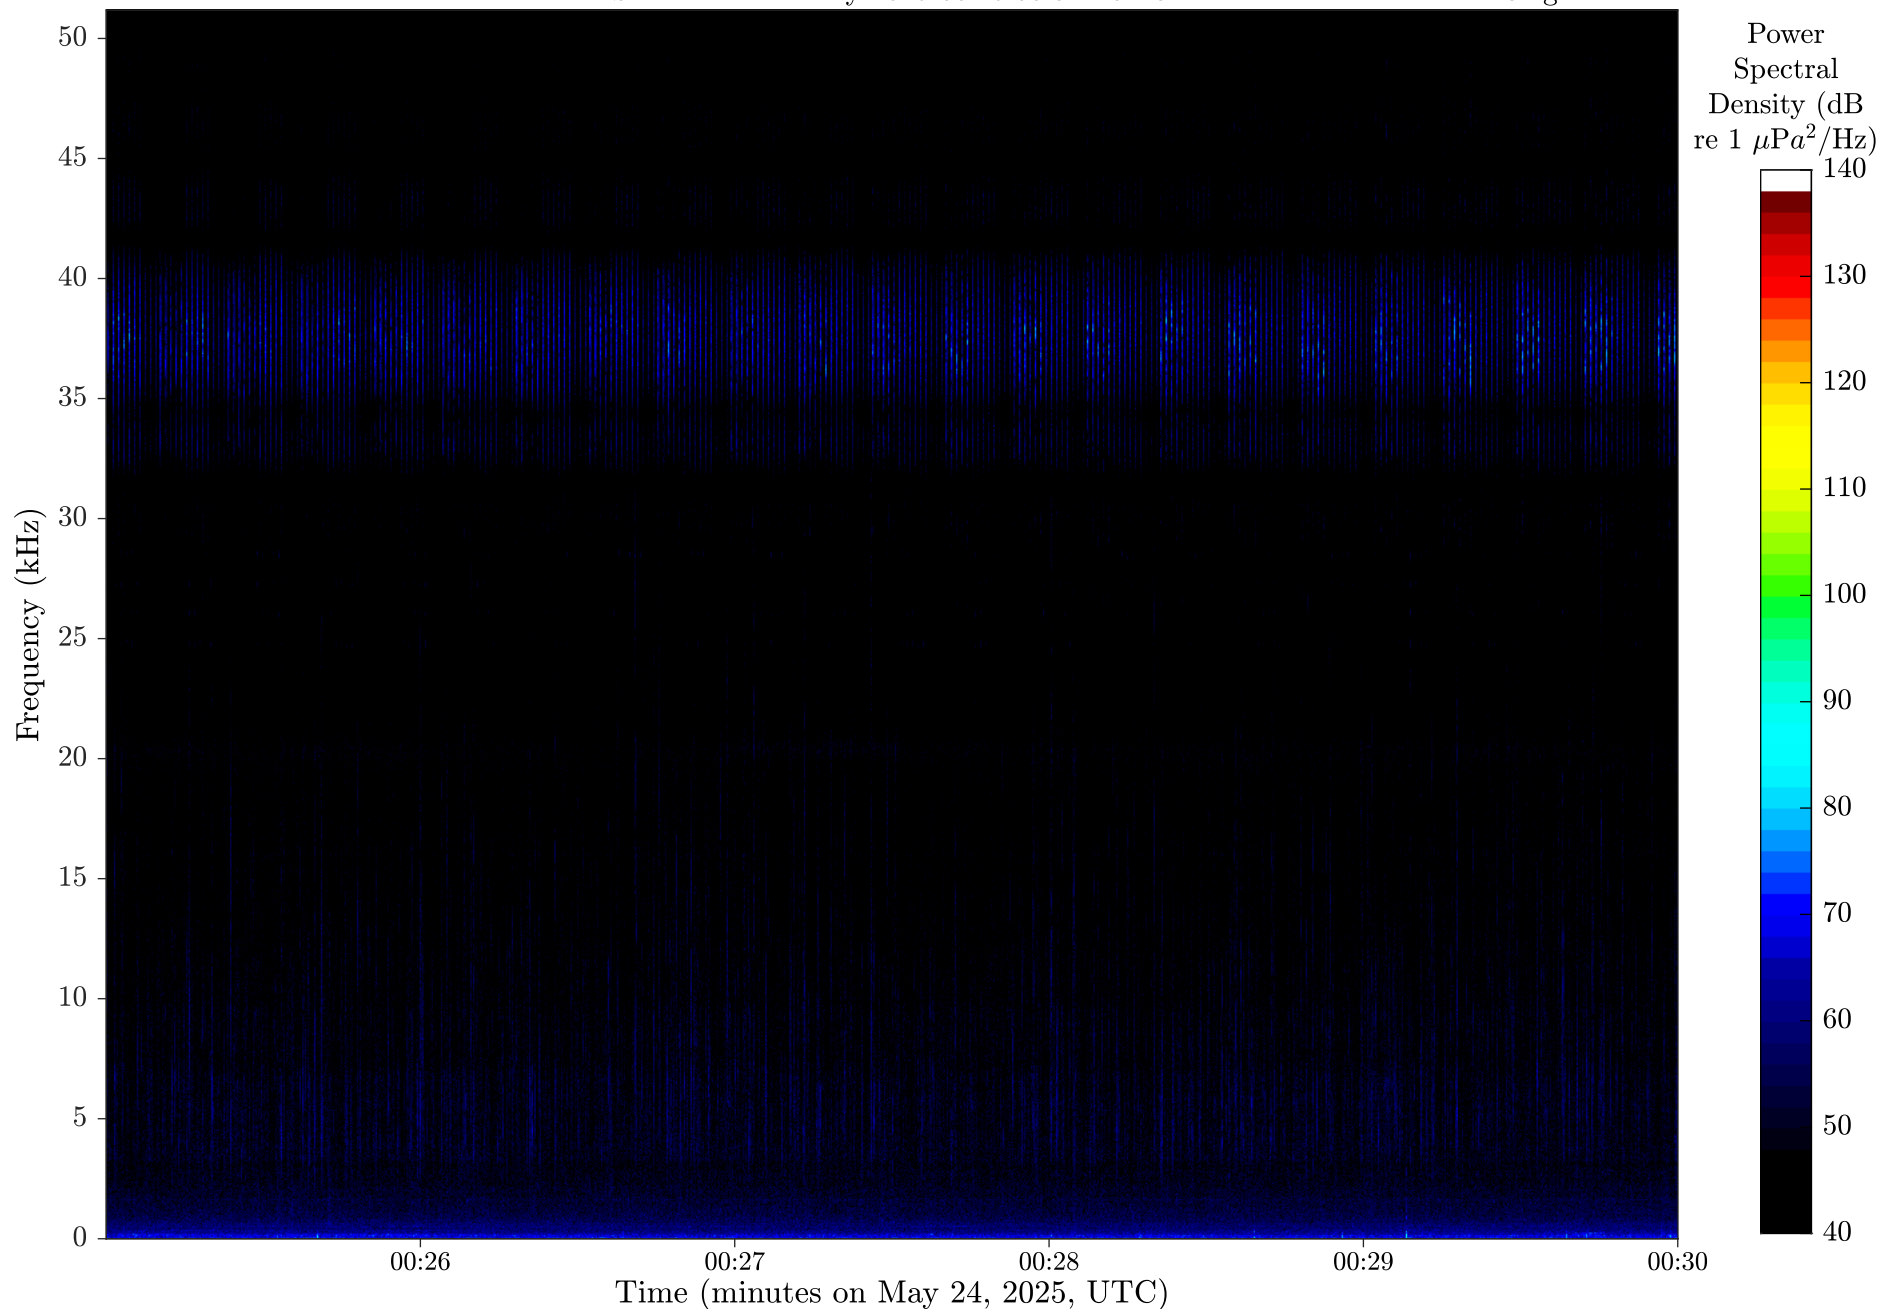

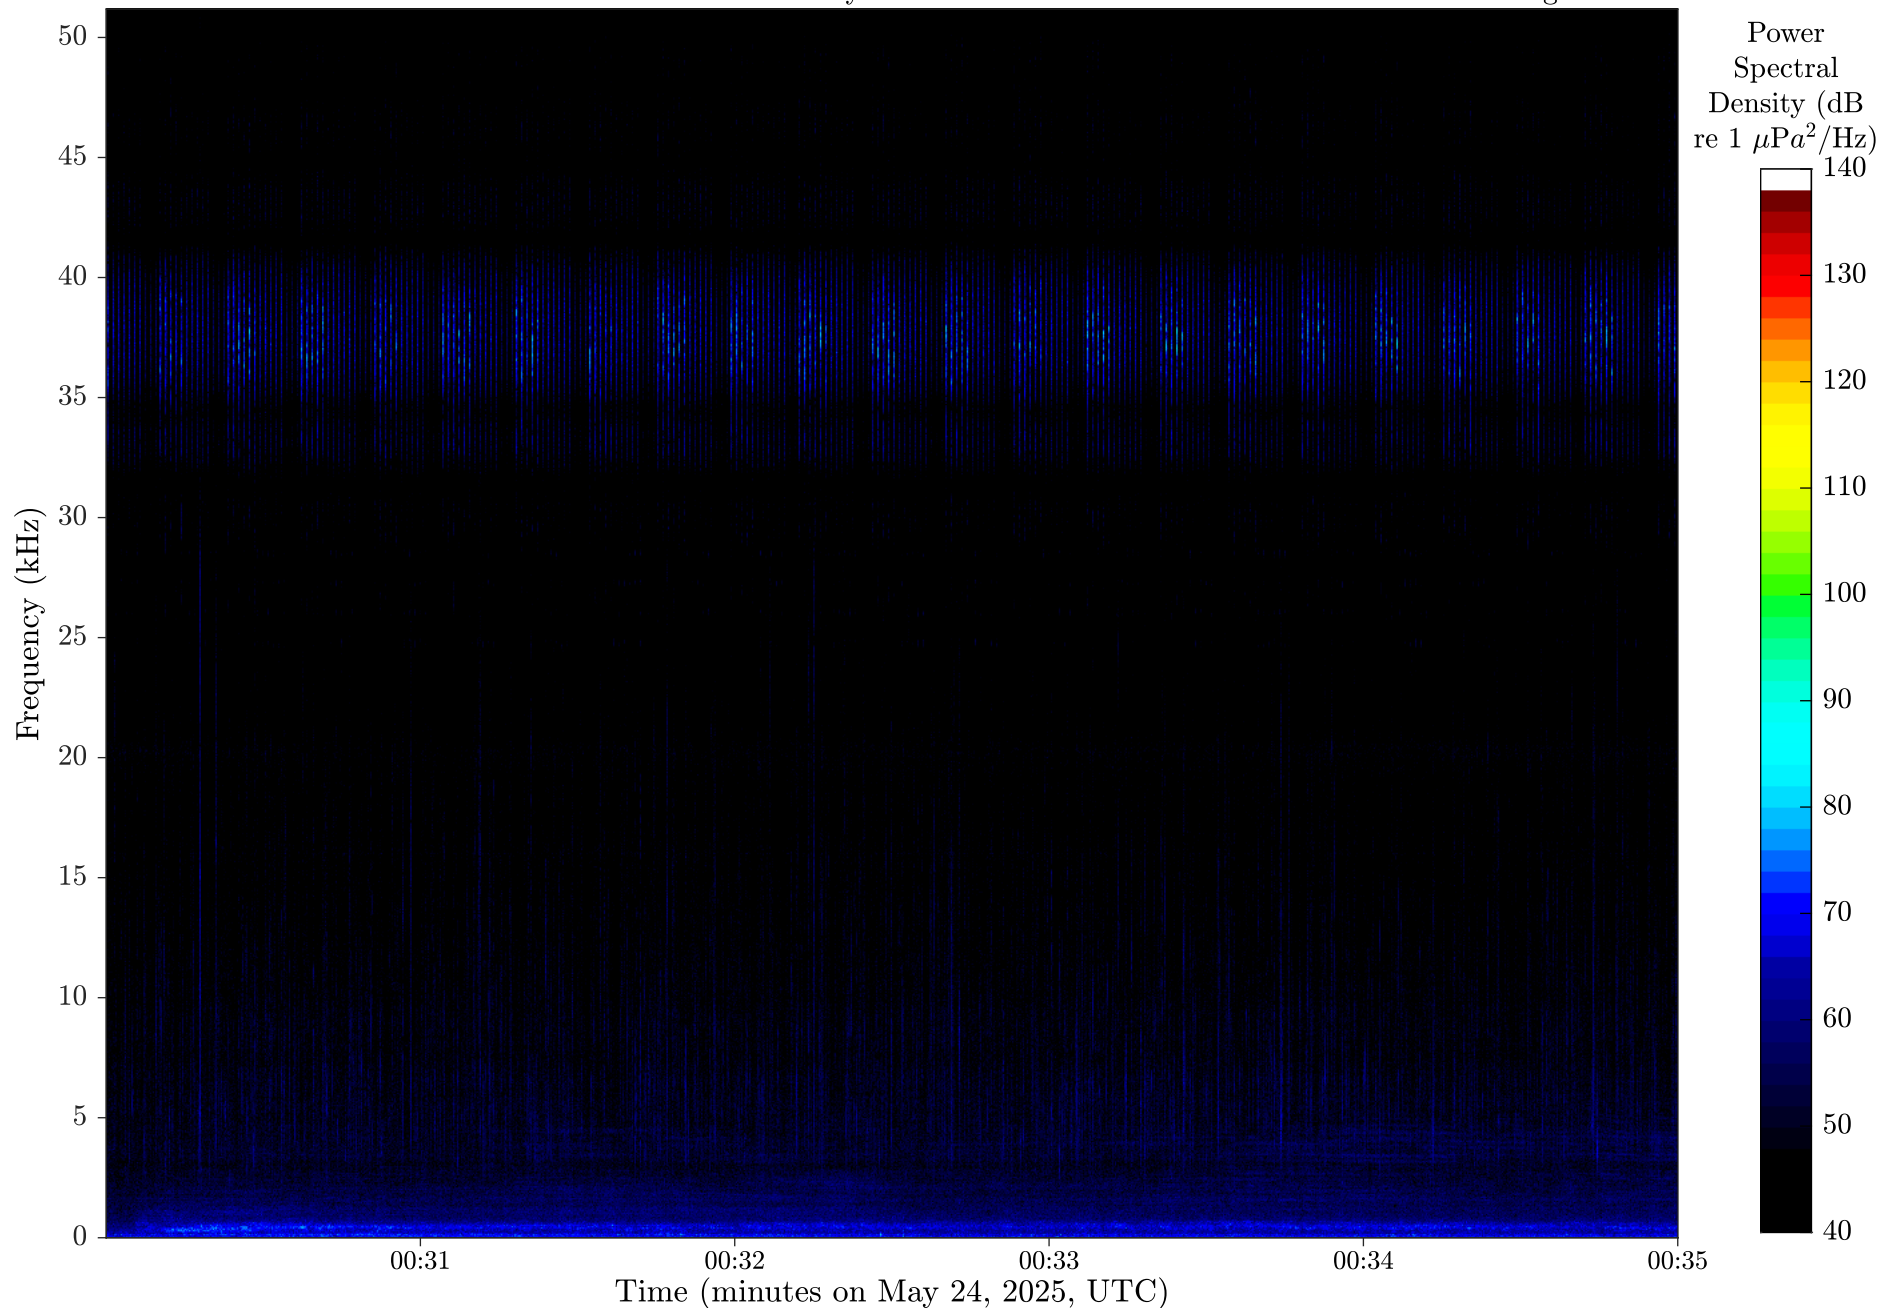


Comments: 33.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:12:59 UTC

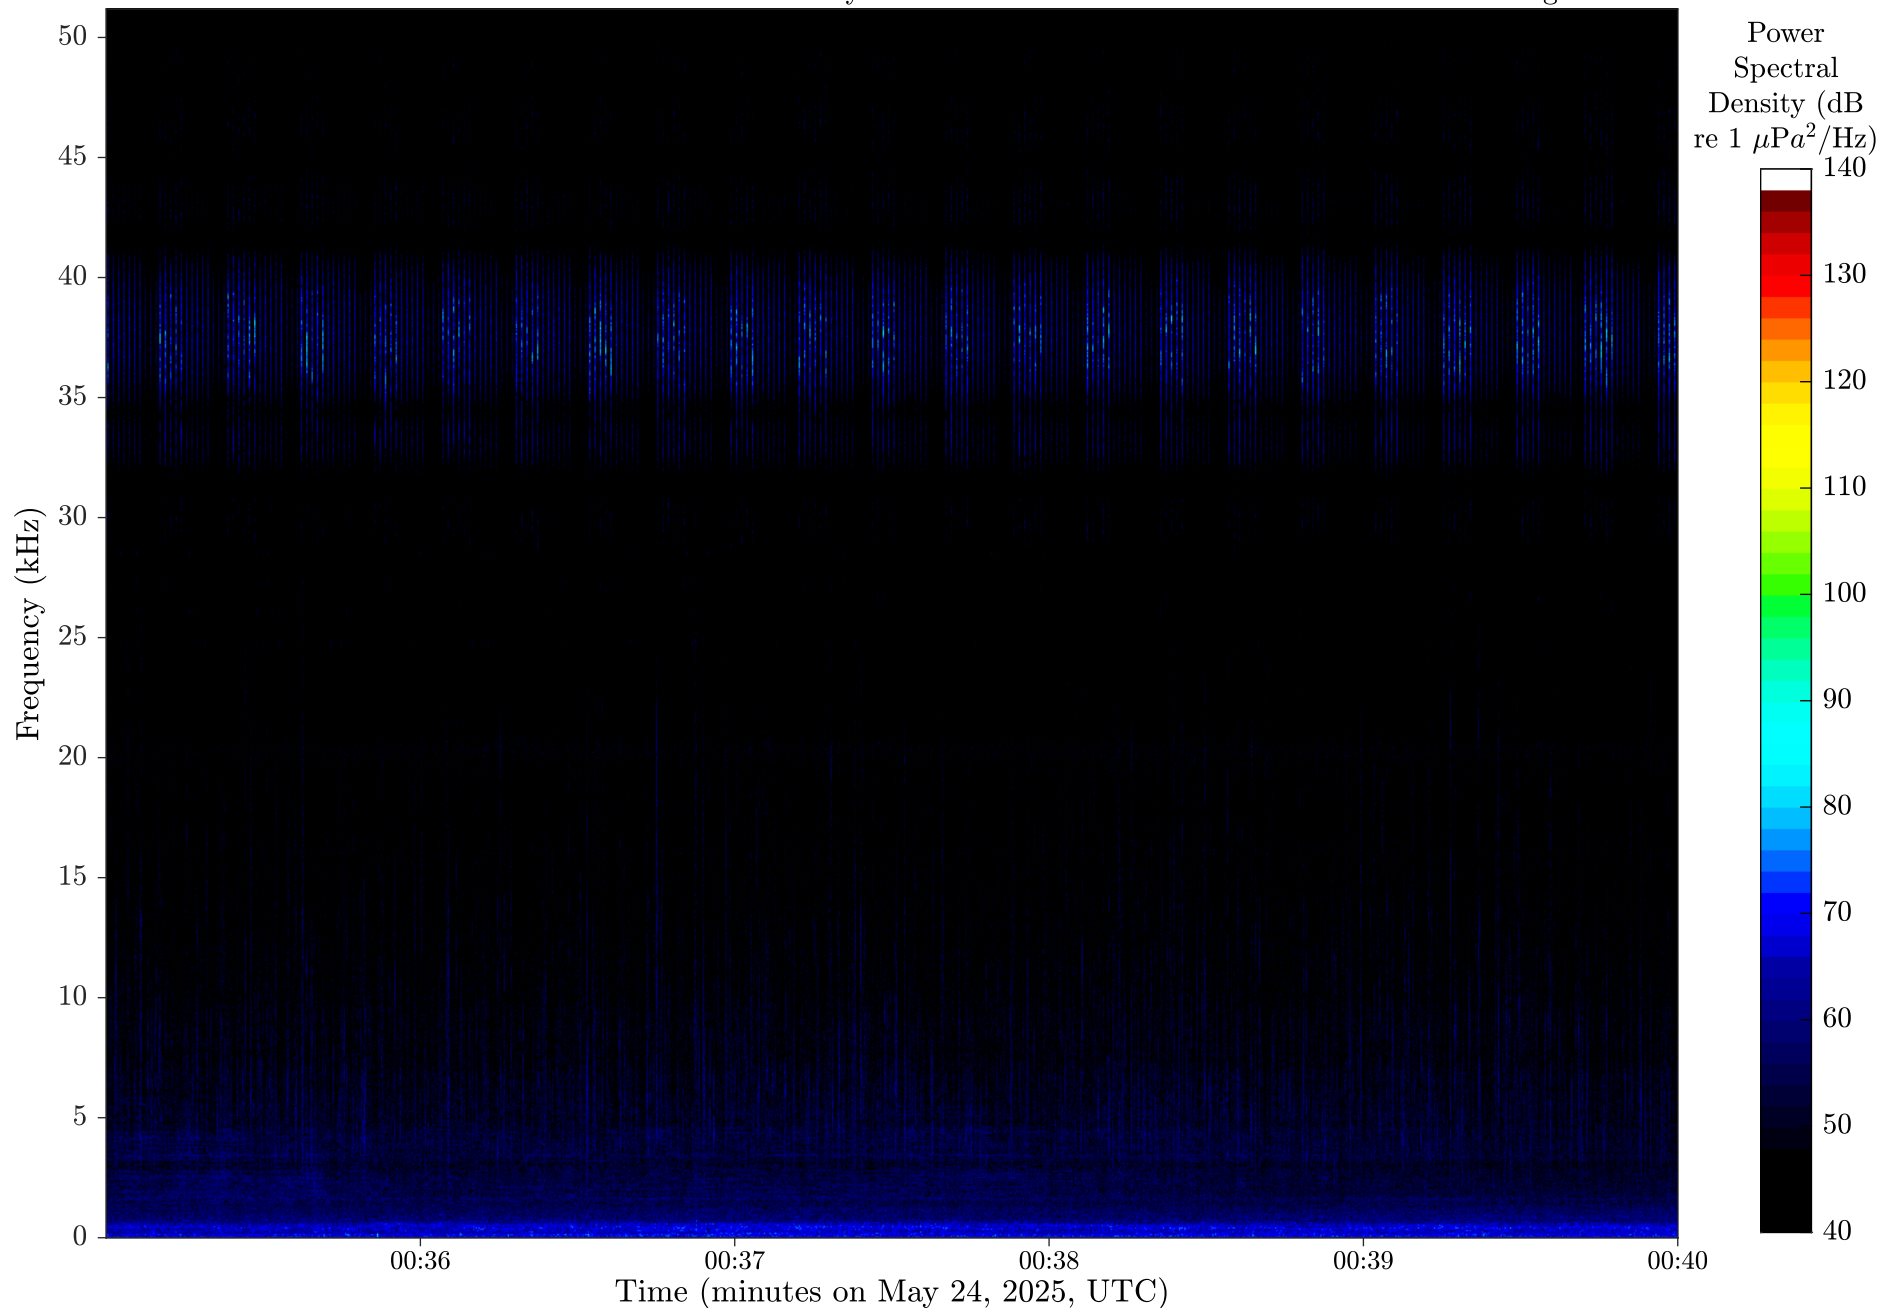

Comments: 34.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:13:06 UTC

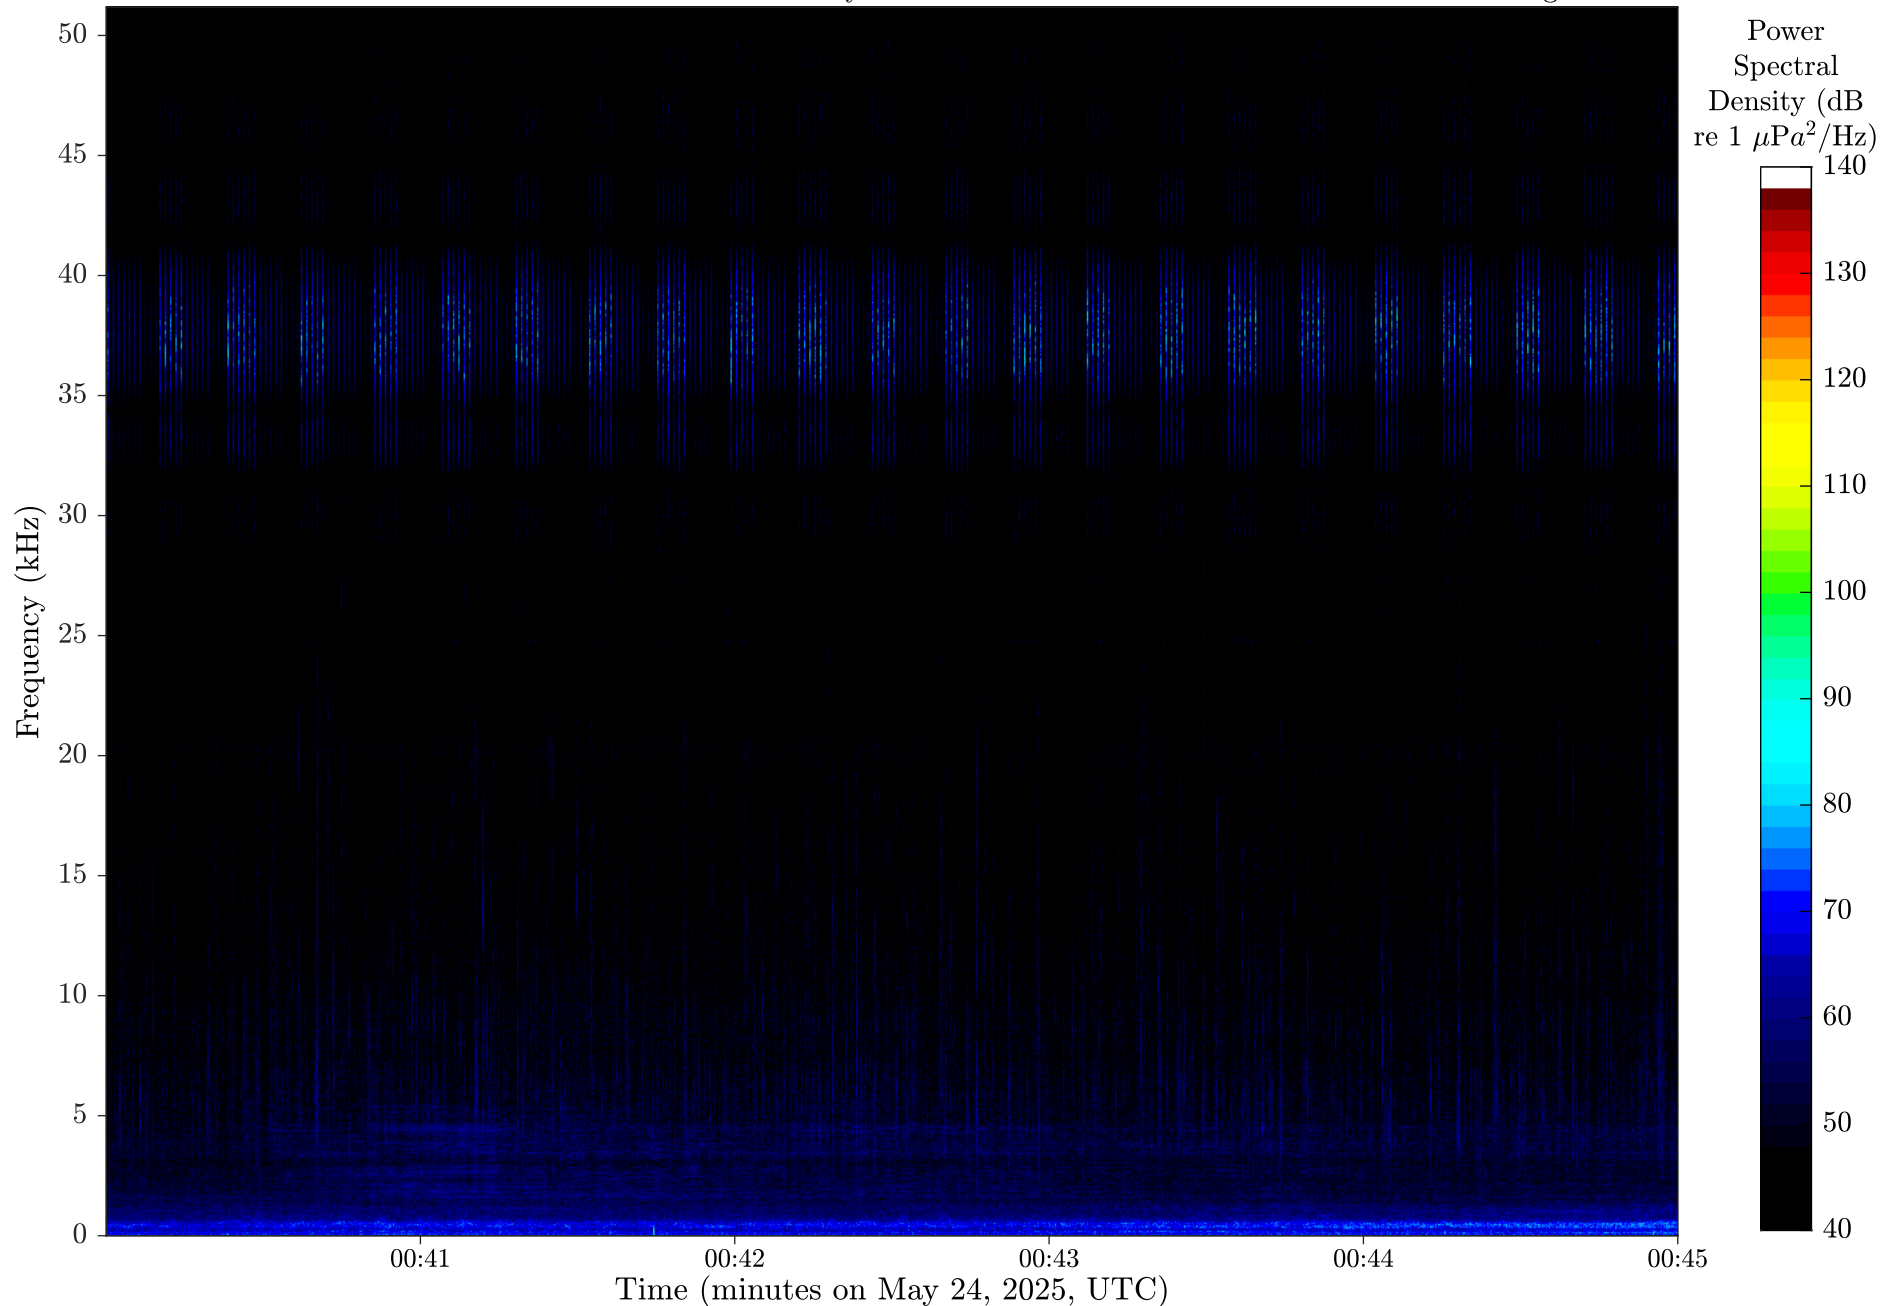

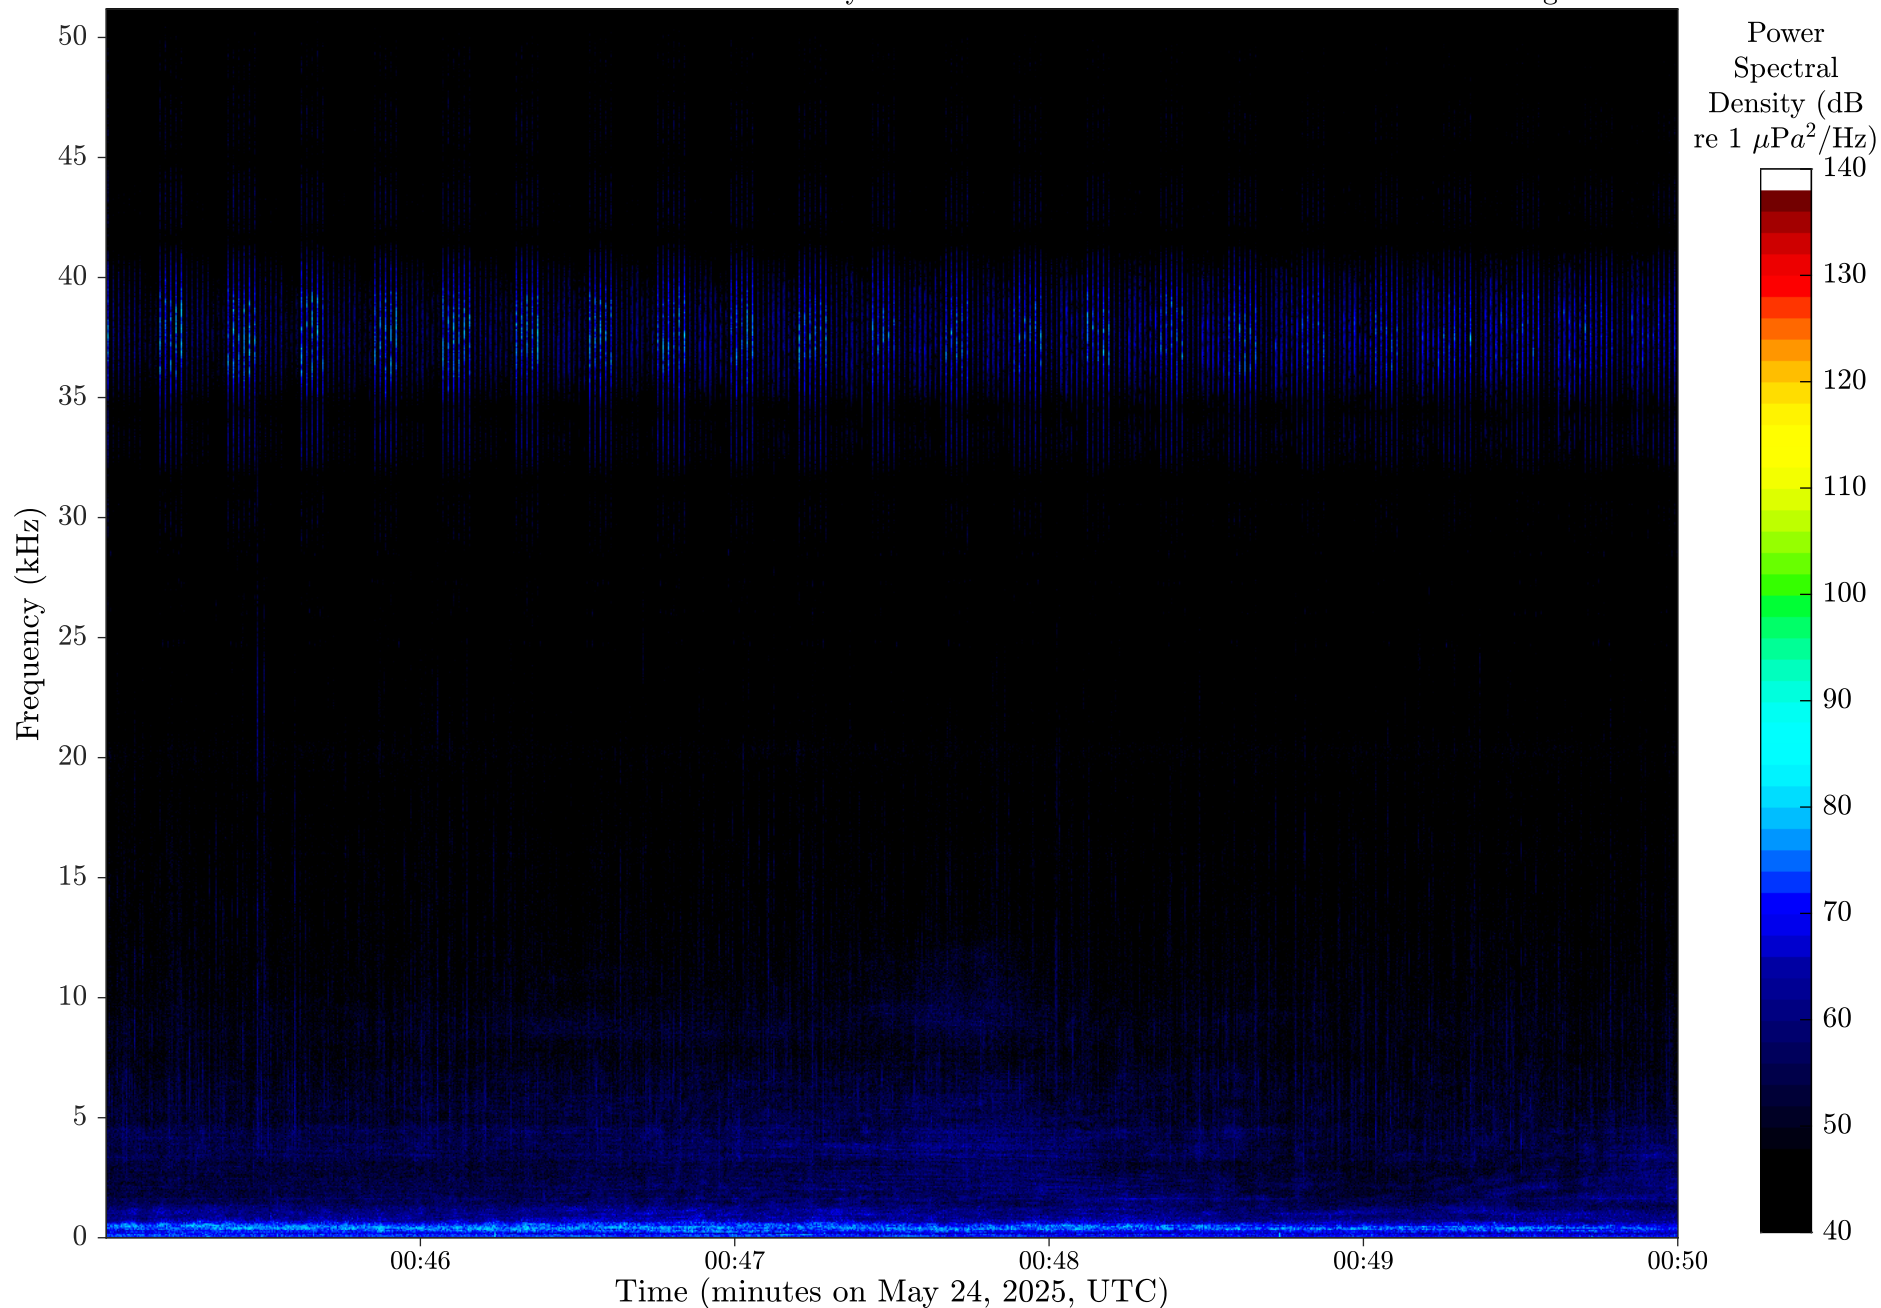


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:13:21 UTC

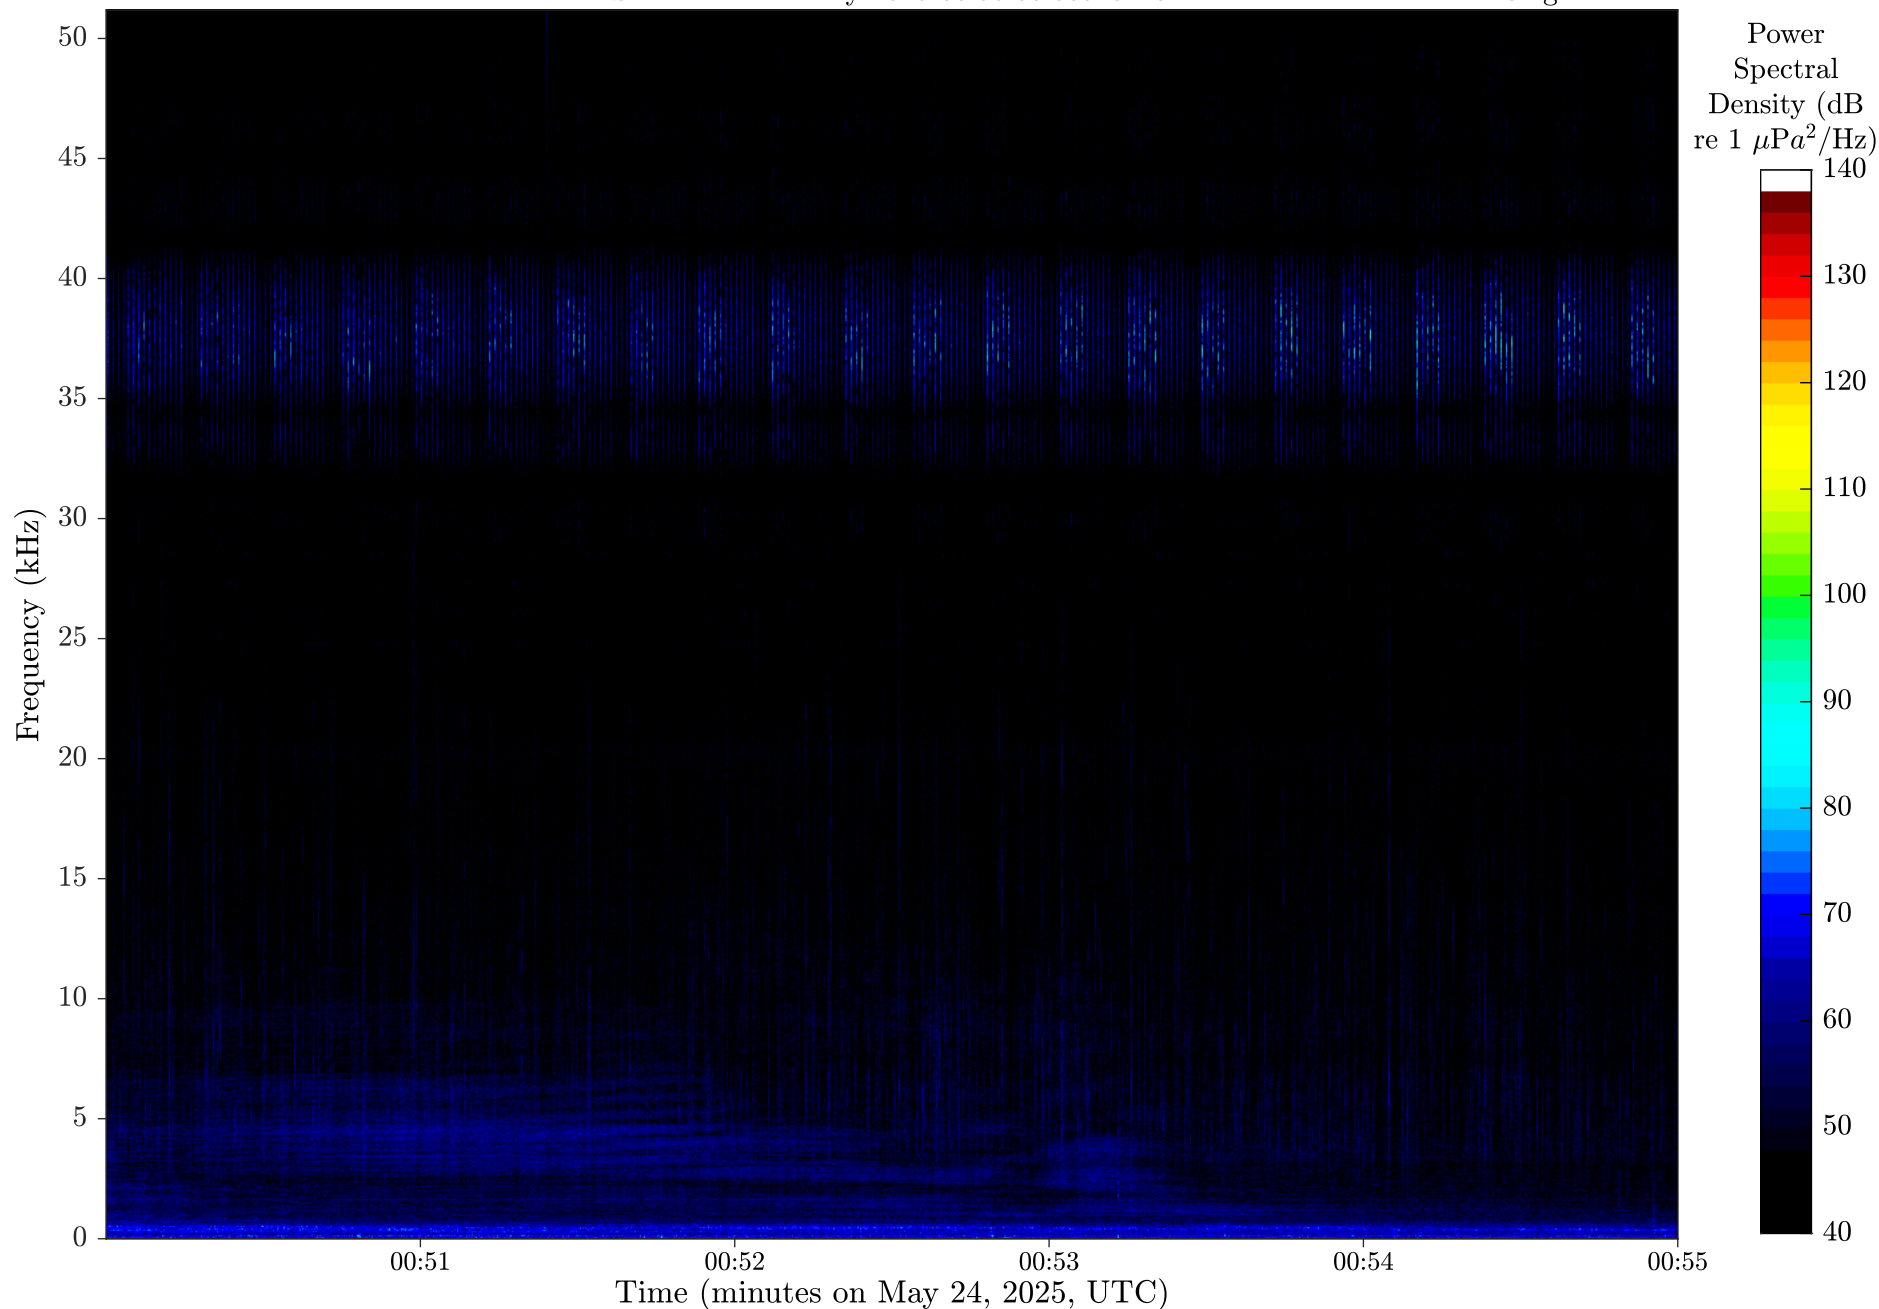


Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:13:28 UTC

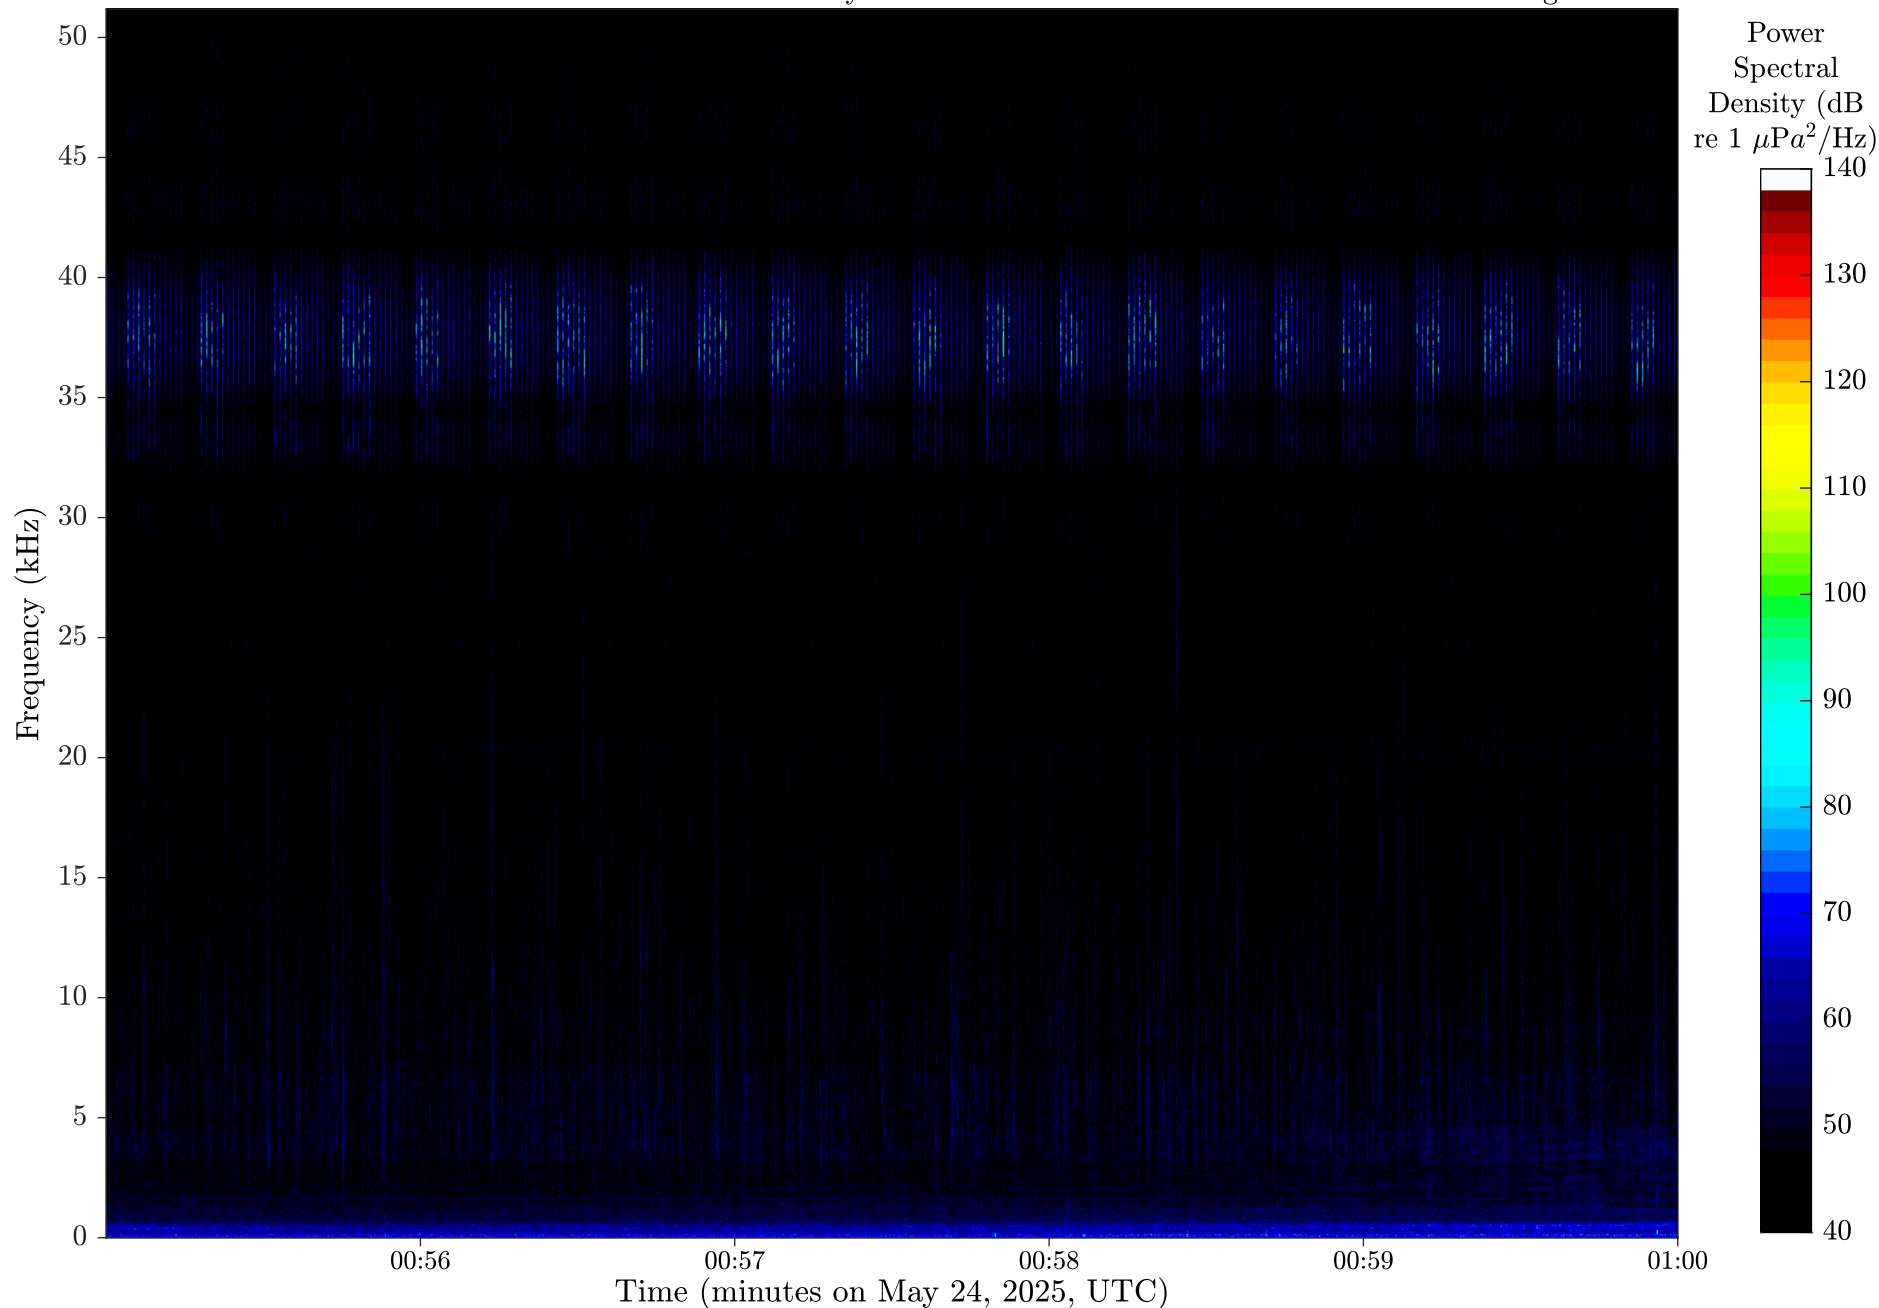


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:13:35 UTC

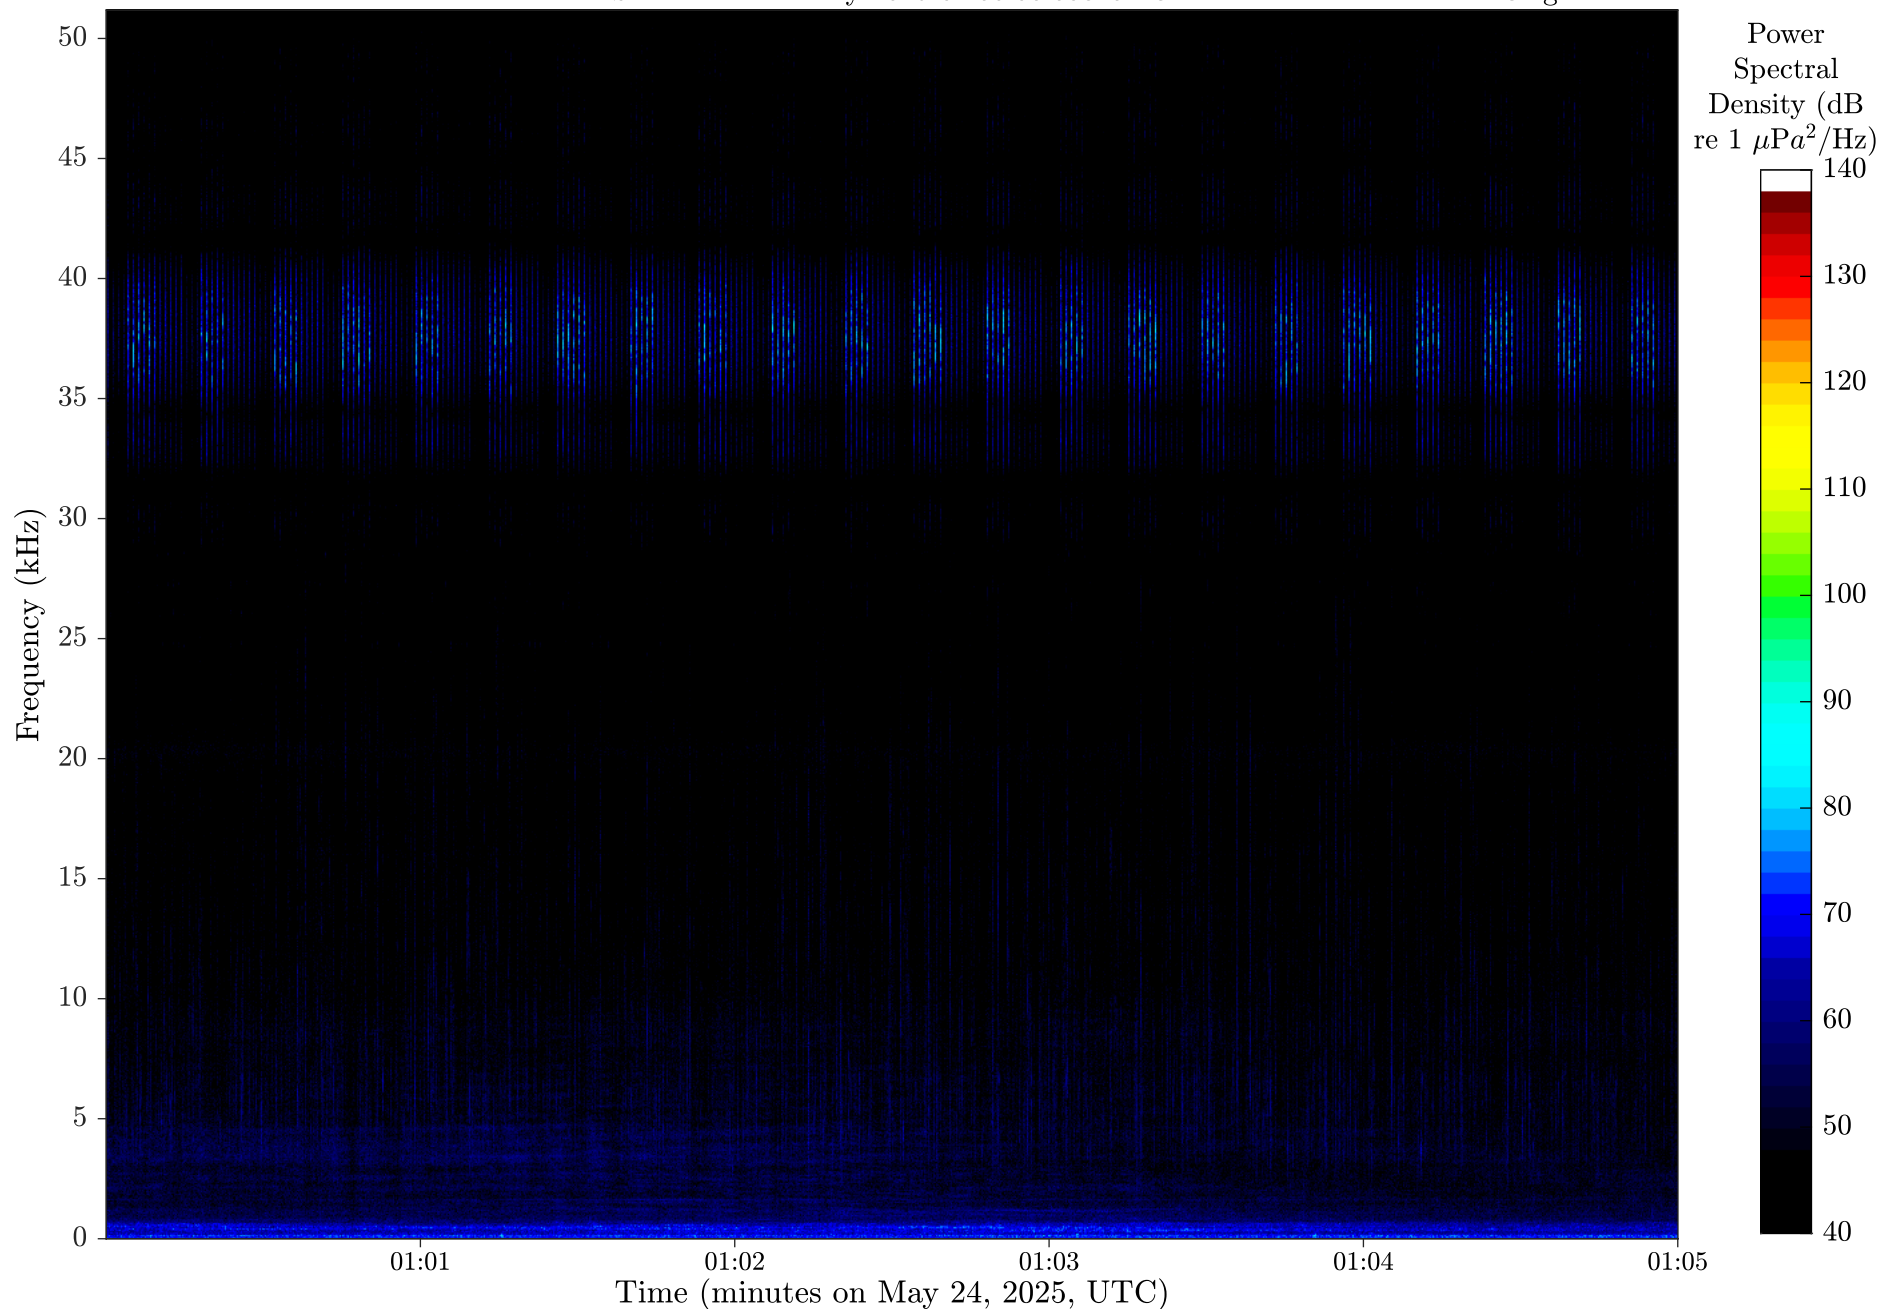


Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:13:42 UTC

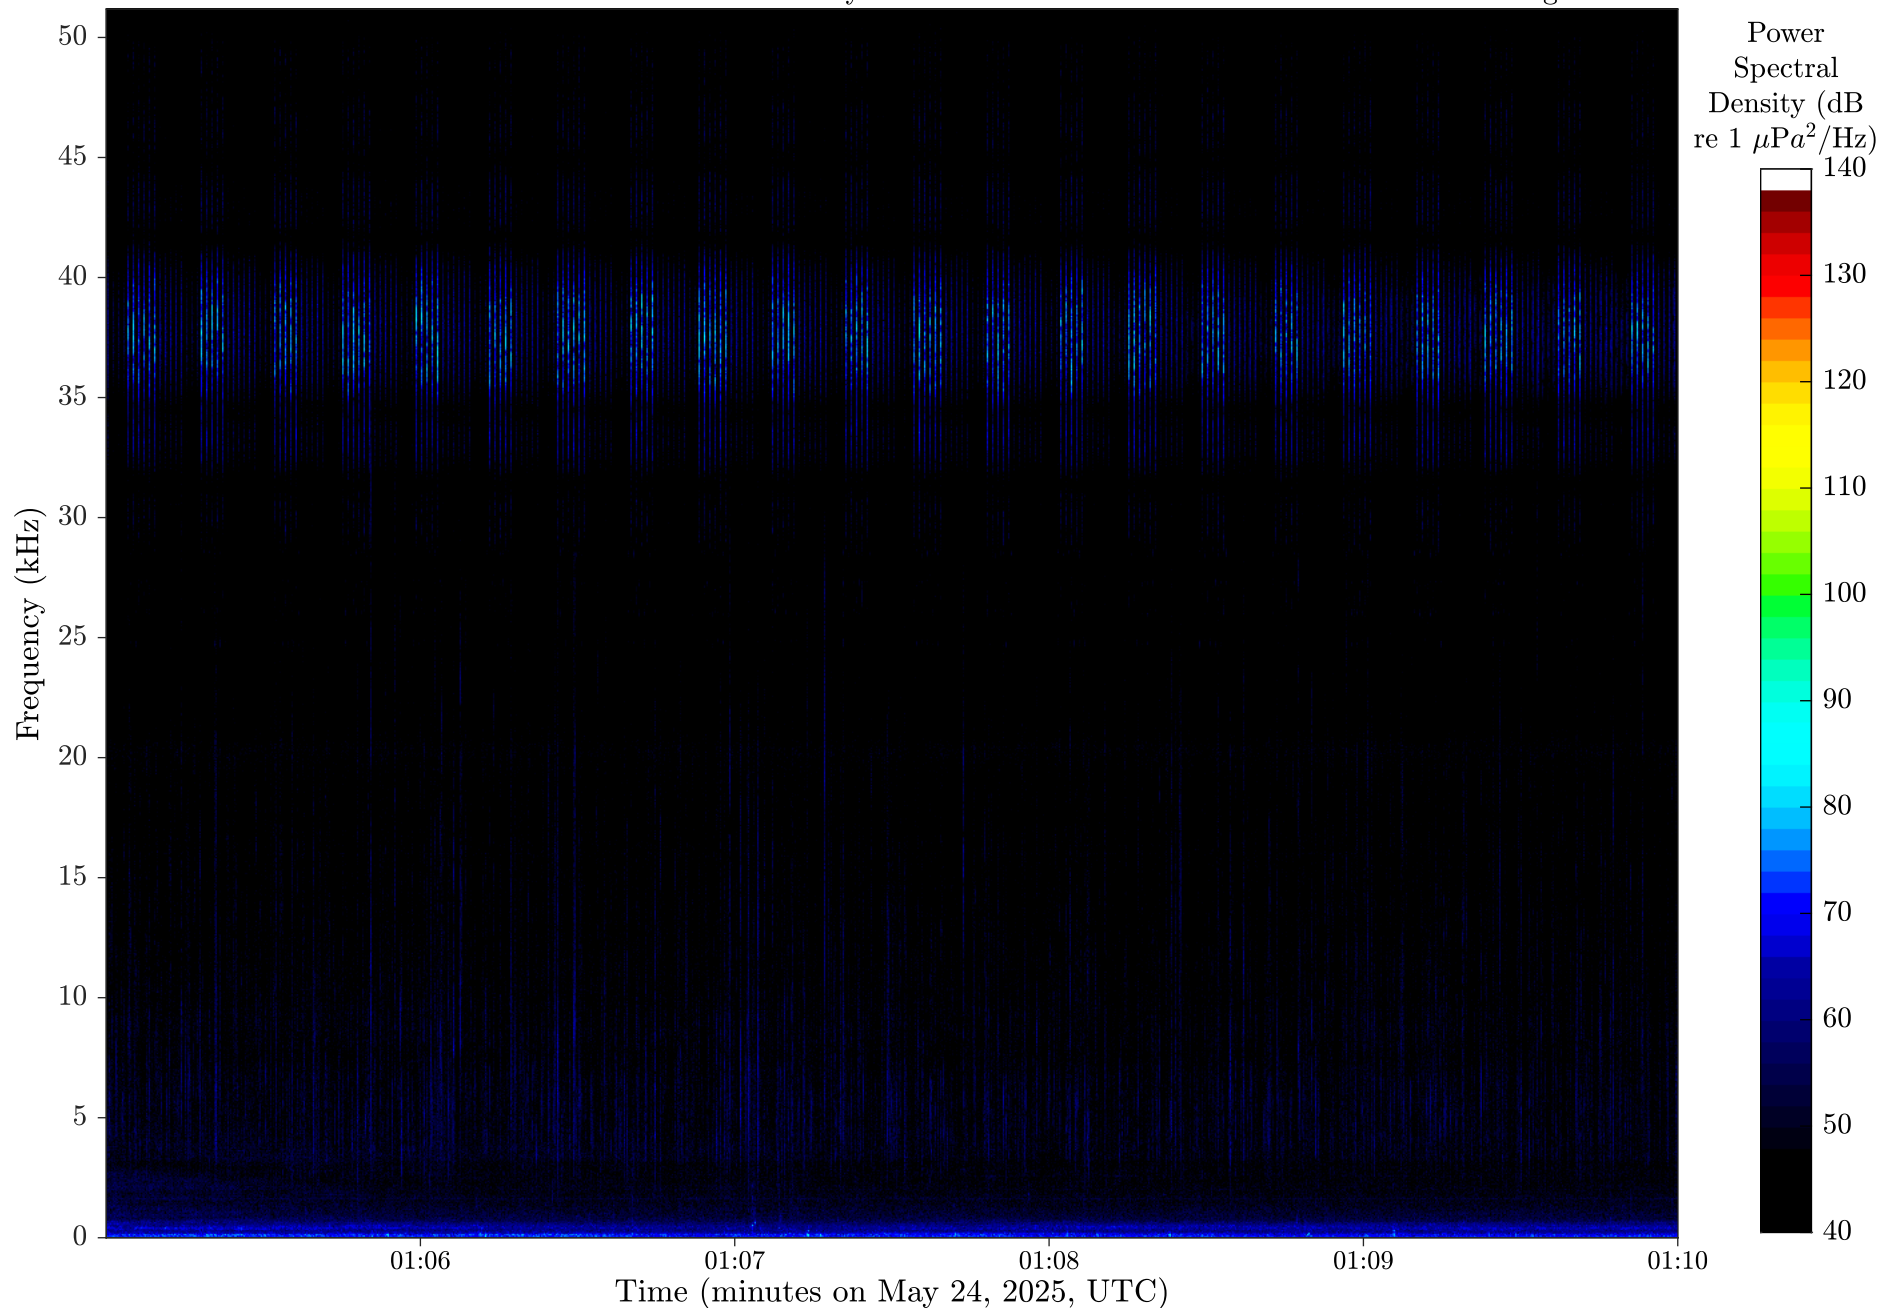


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:13:49 UTC

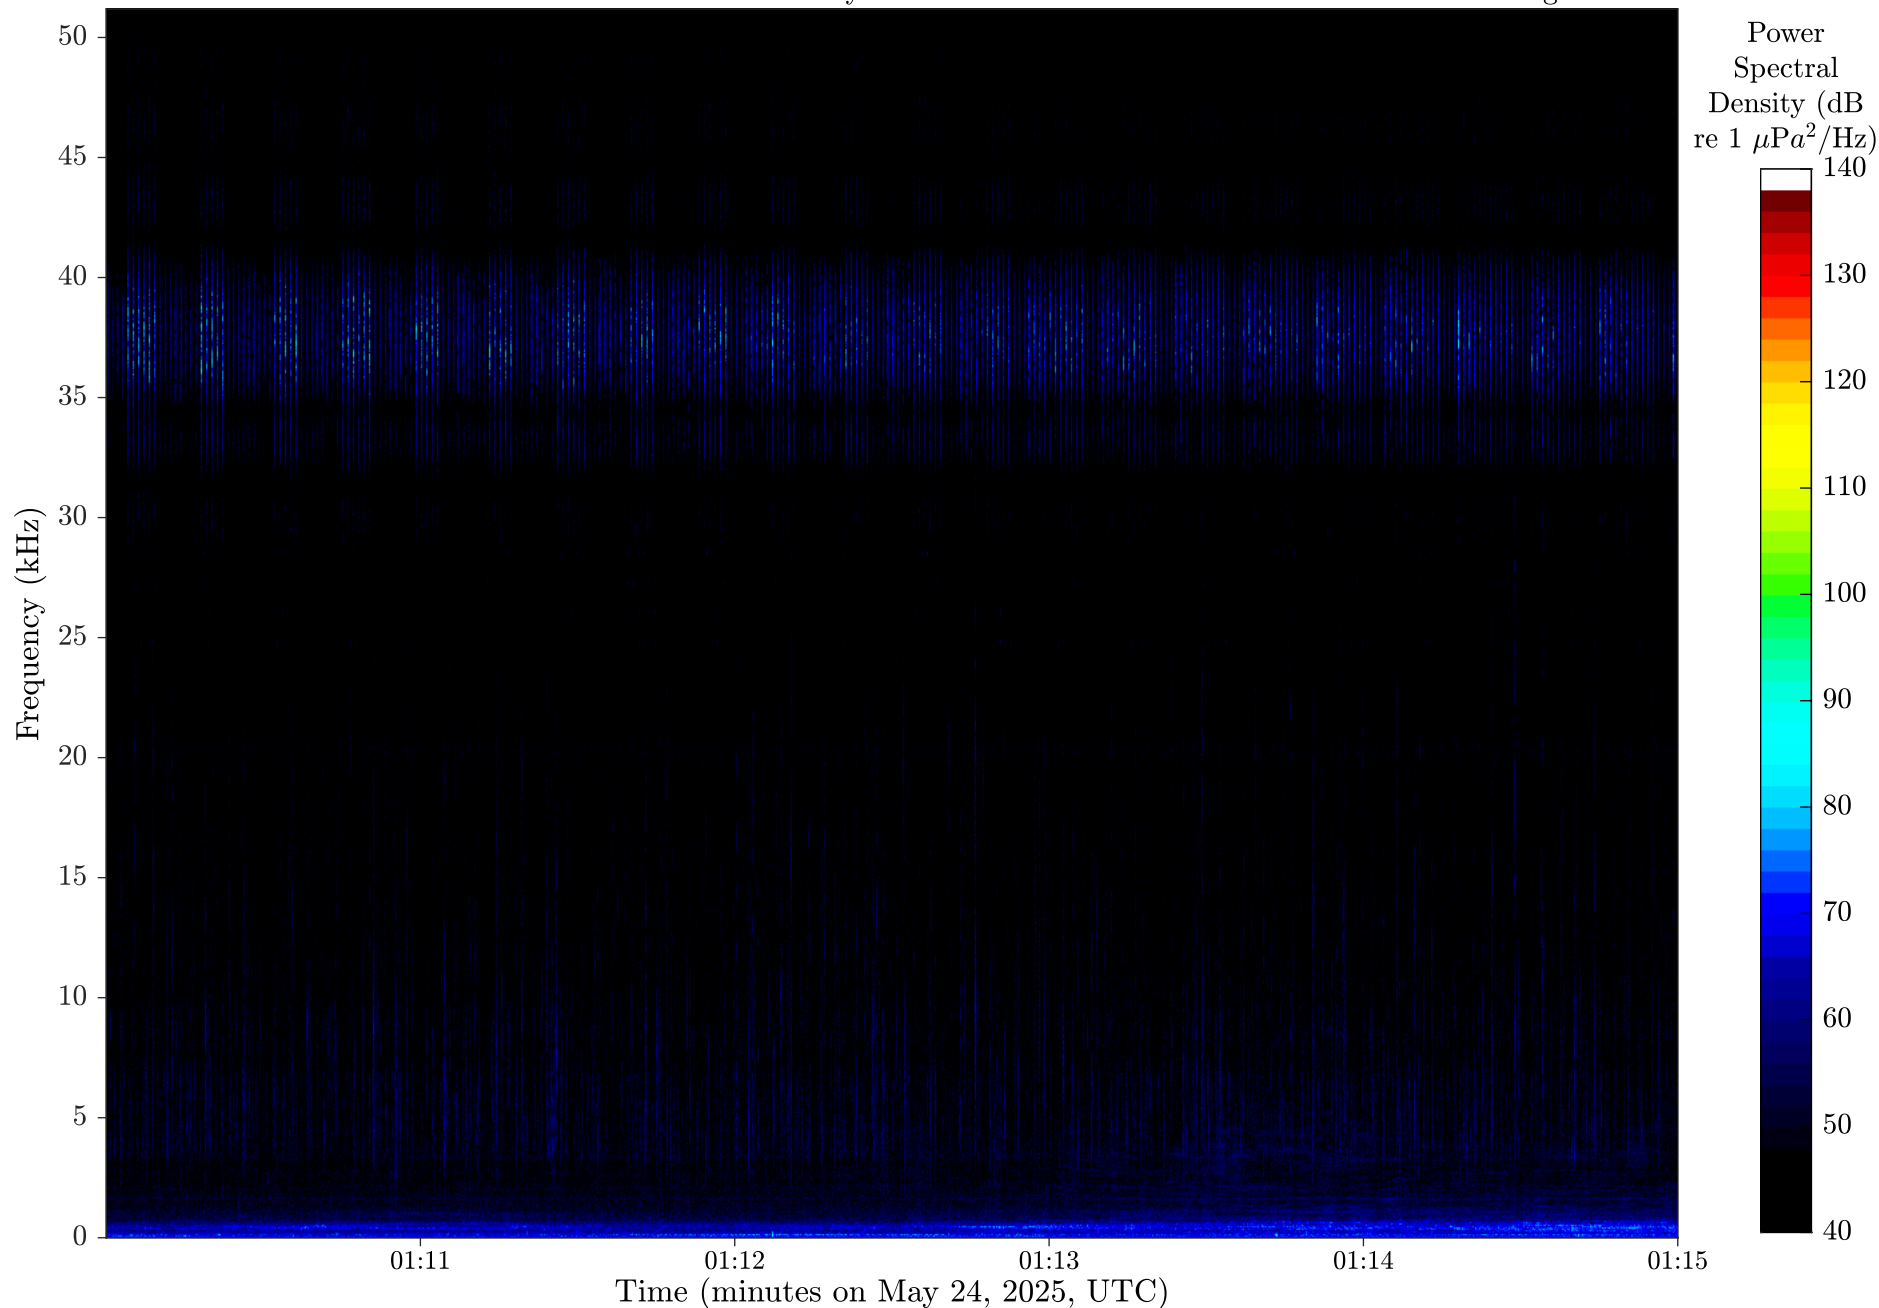


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:13:56 UTC

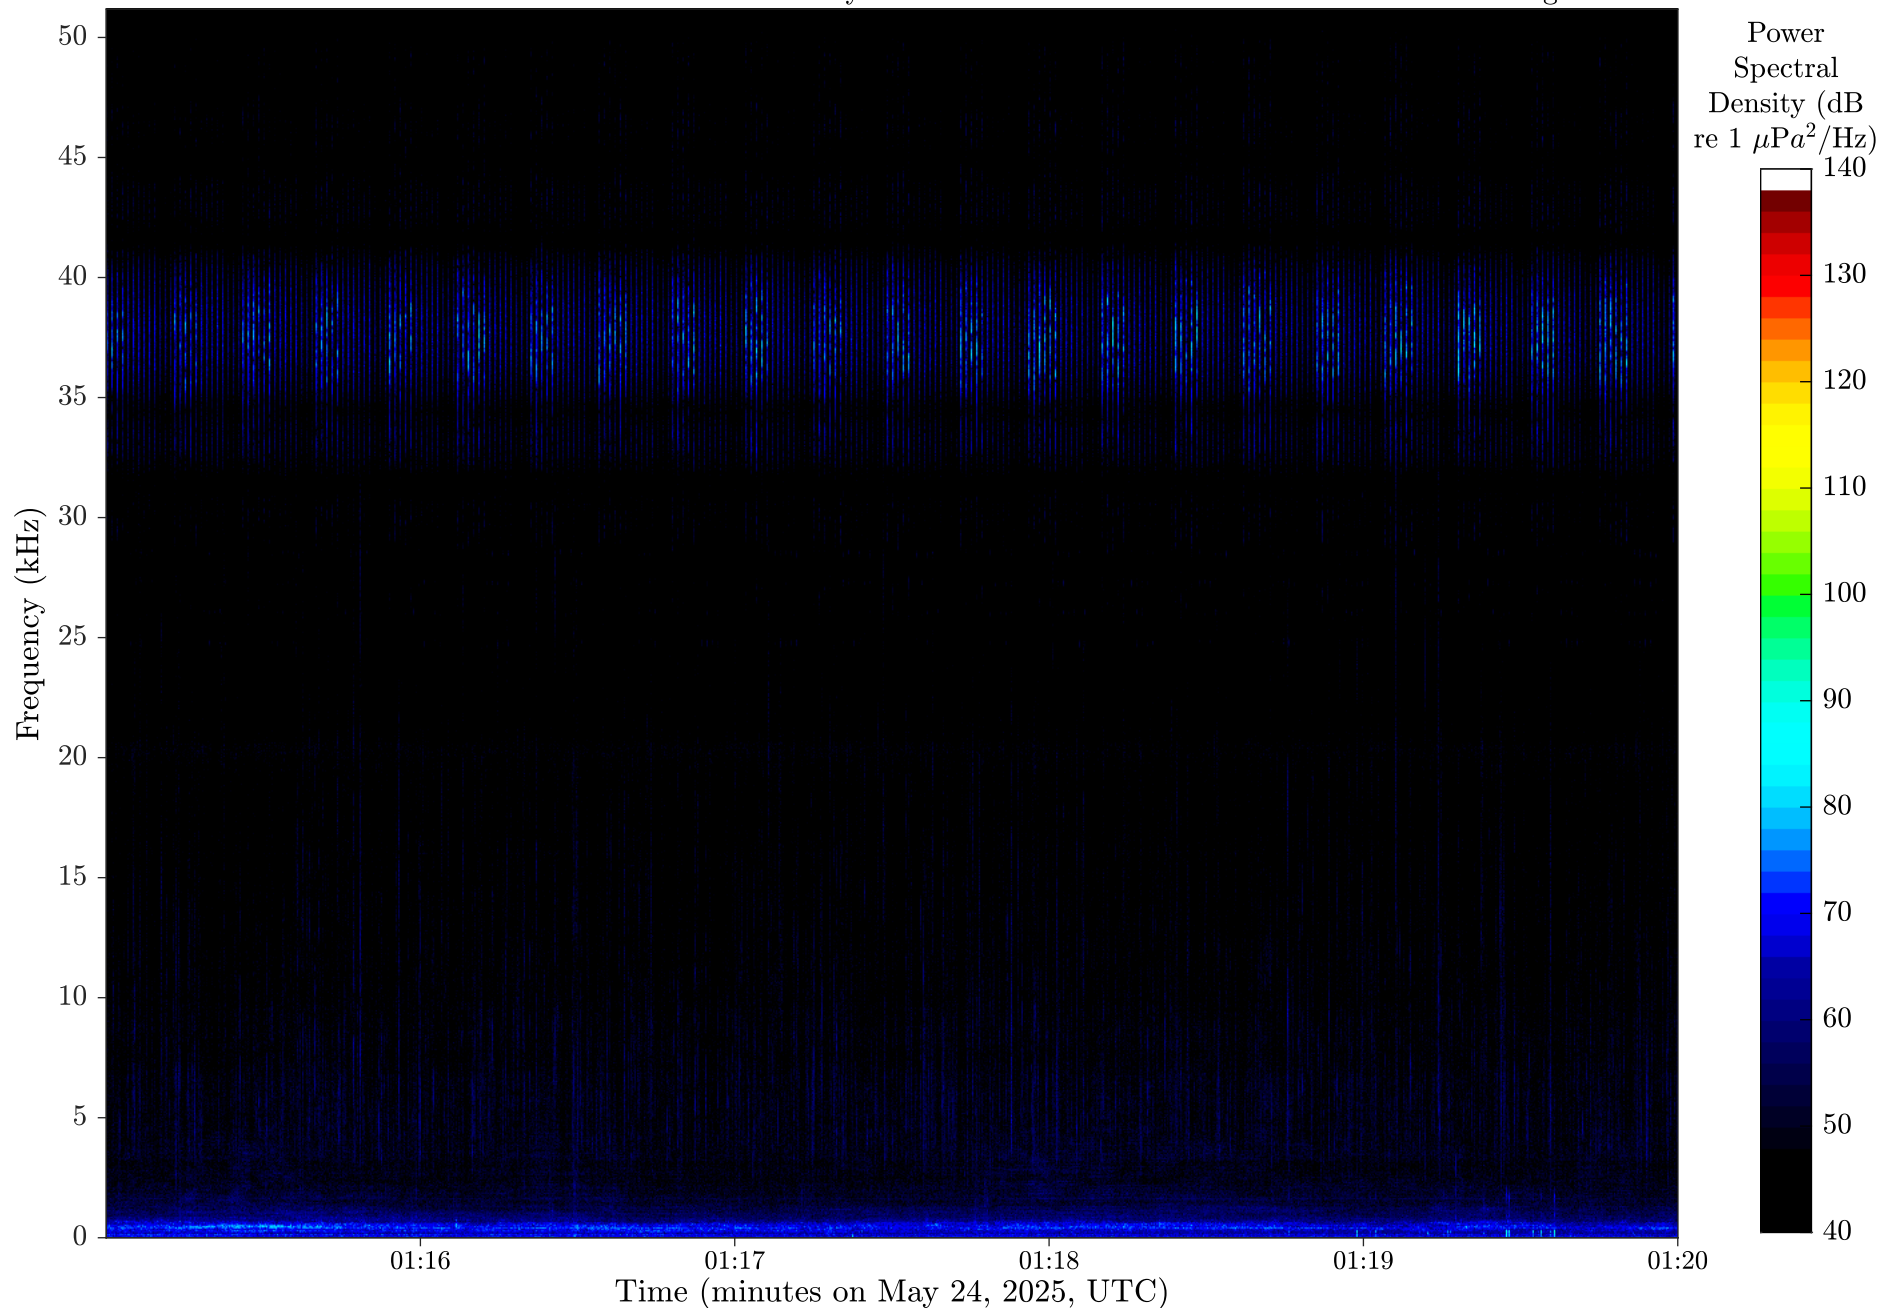


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:14:03 UTC

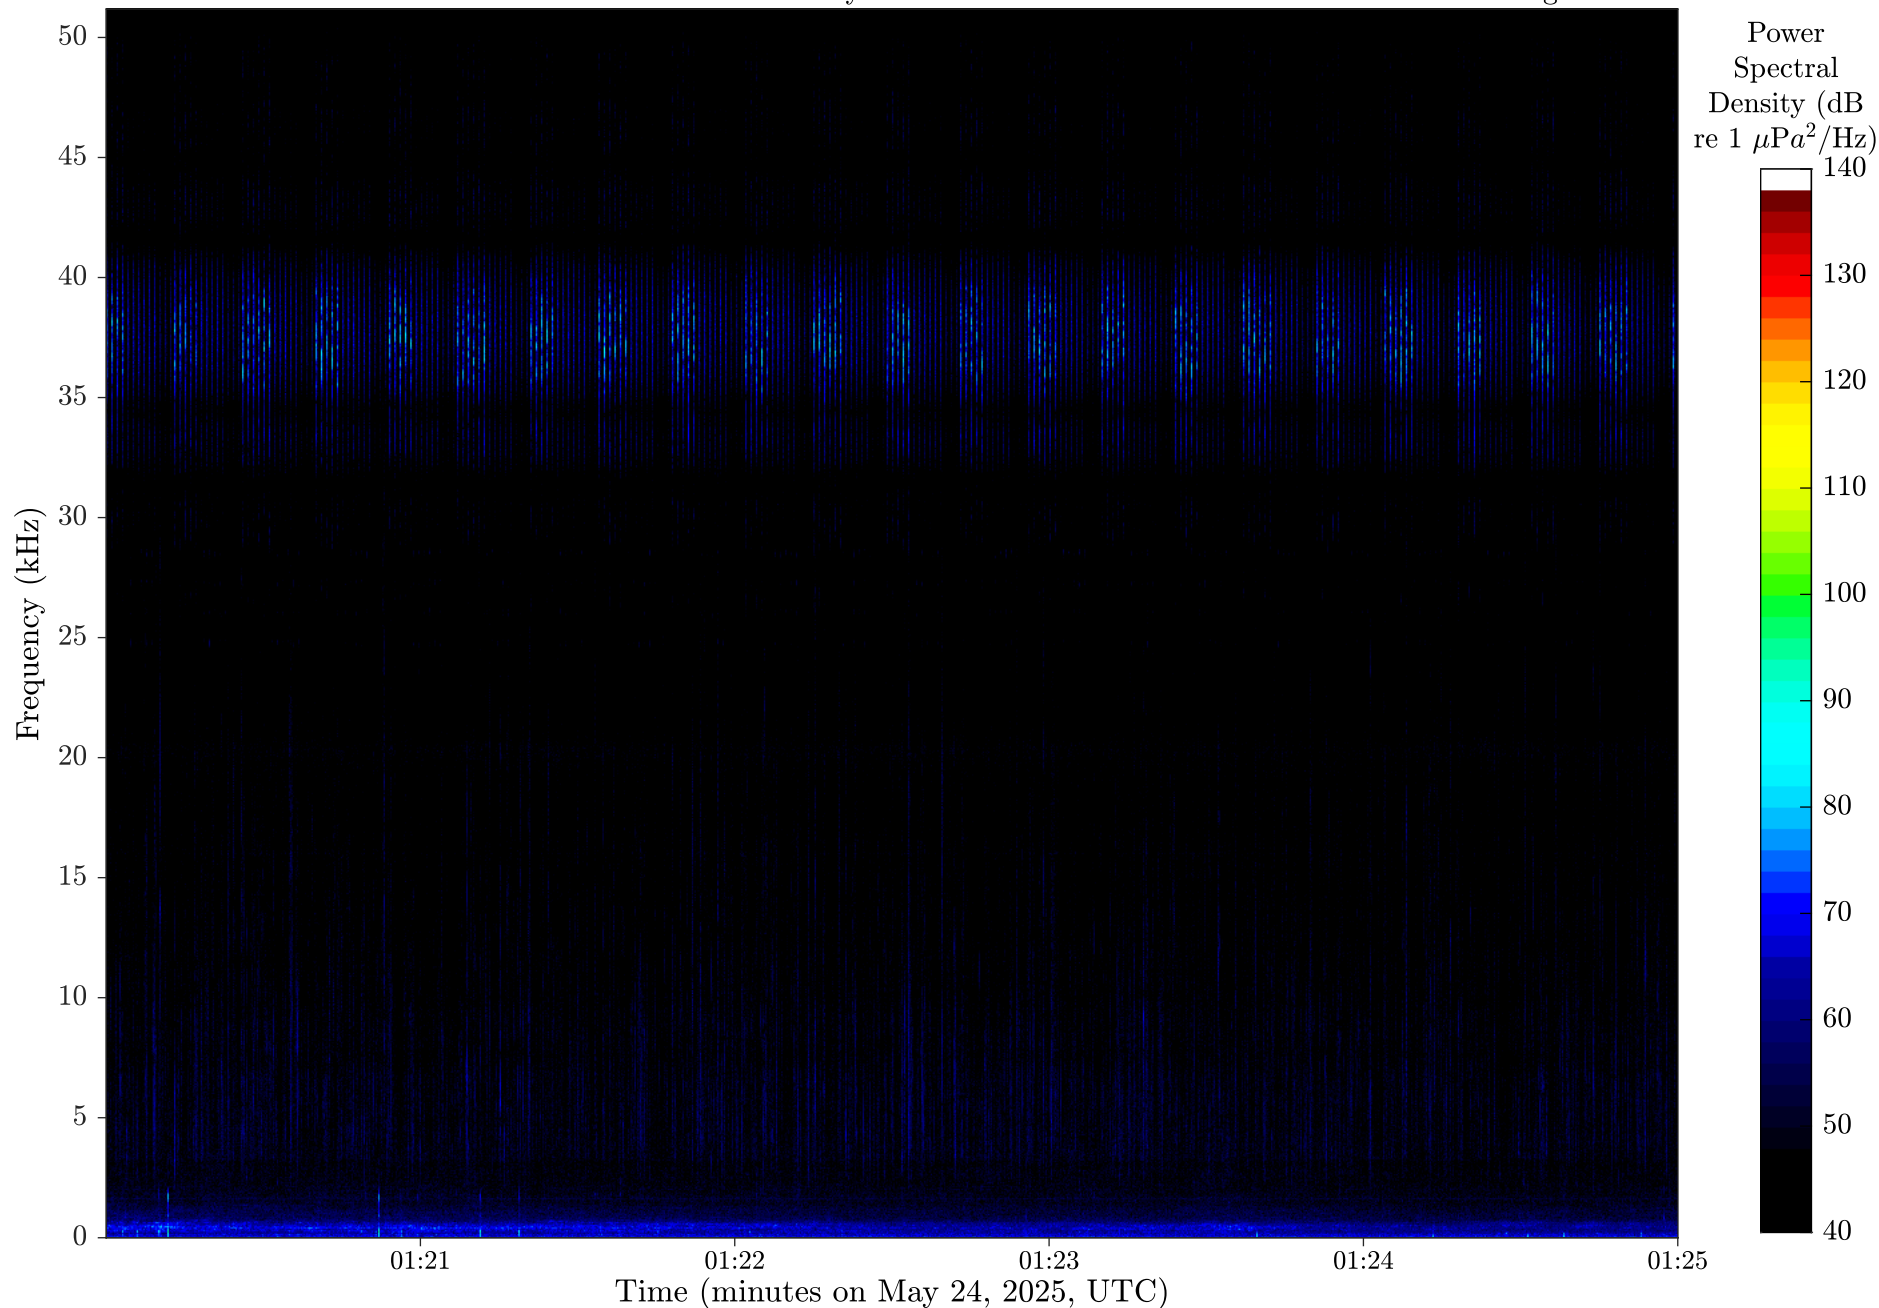


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:14:10 UTC

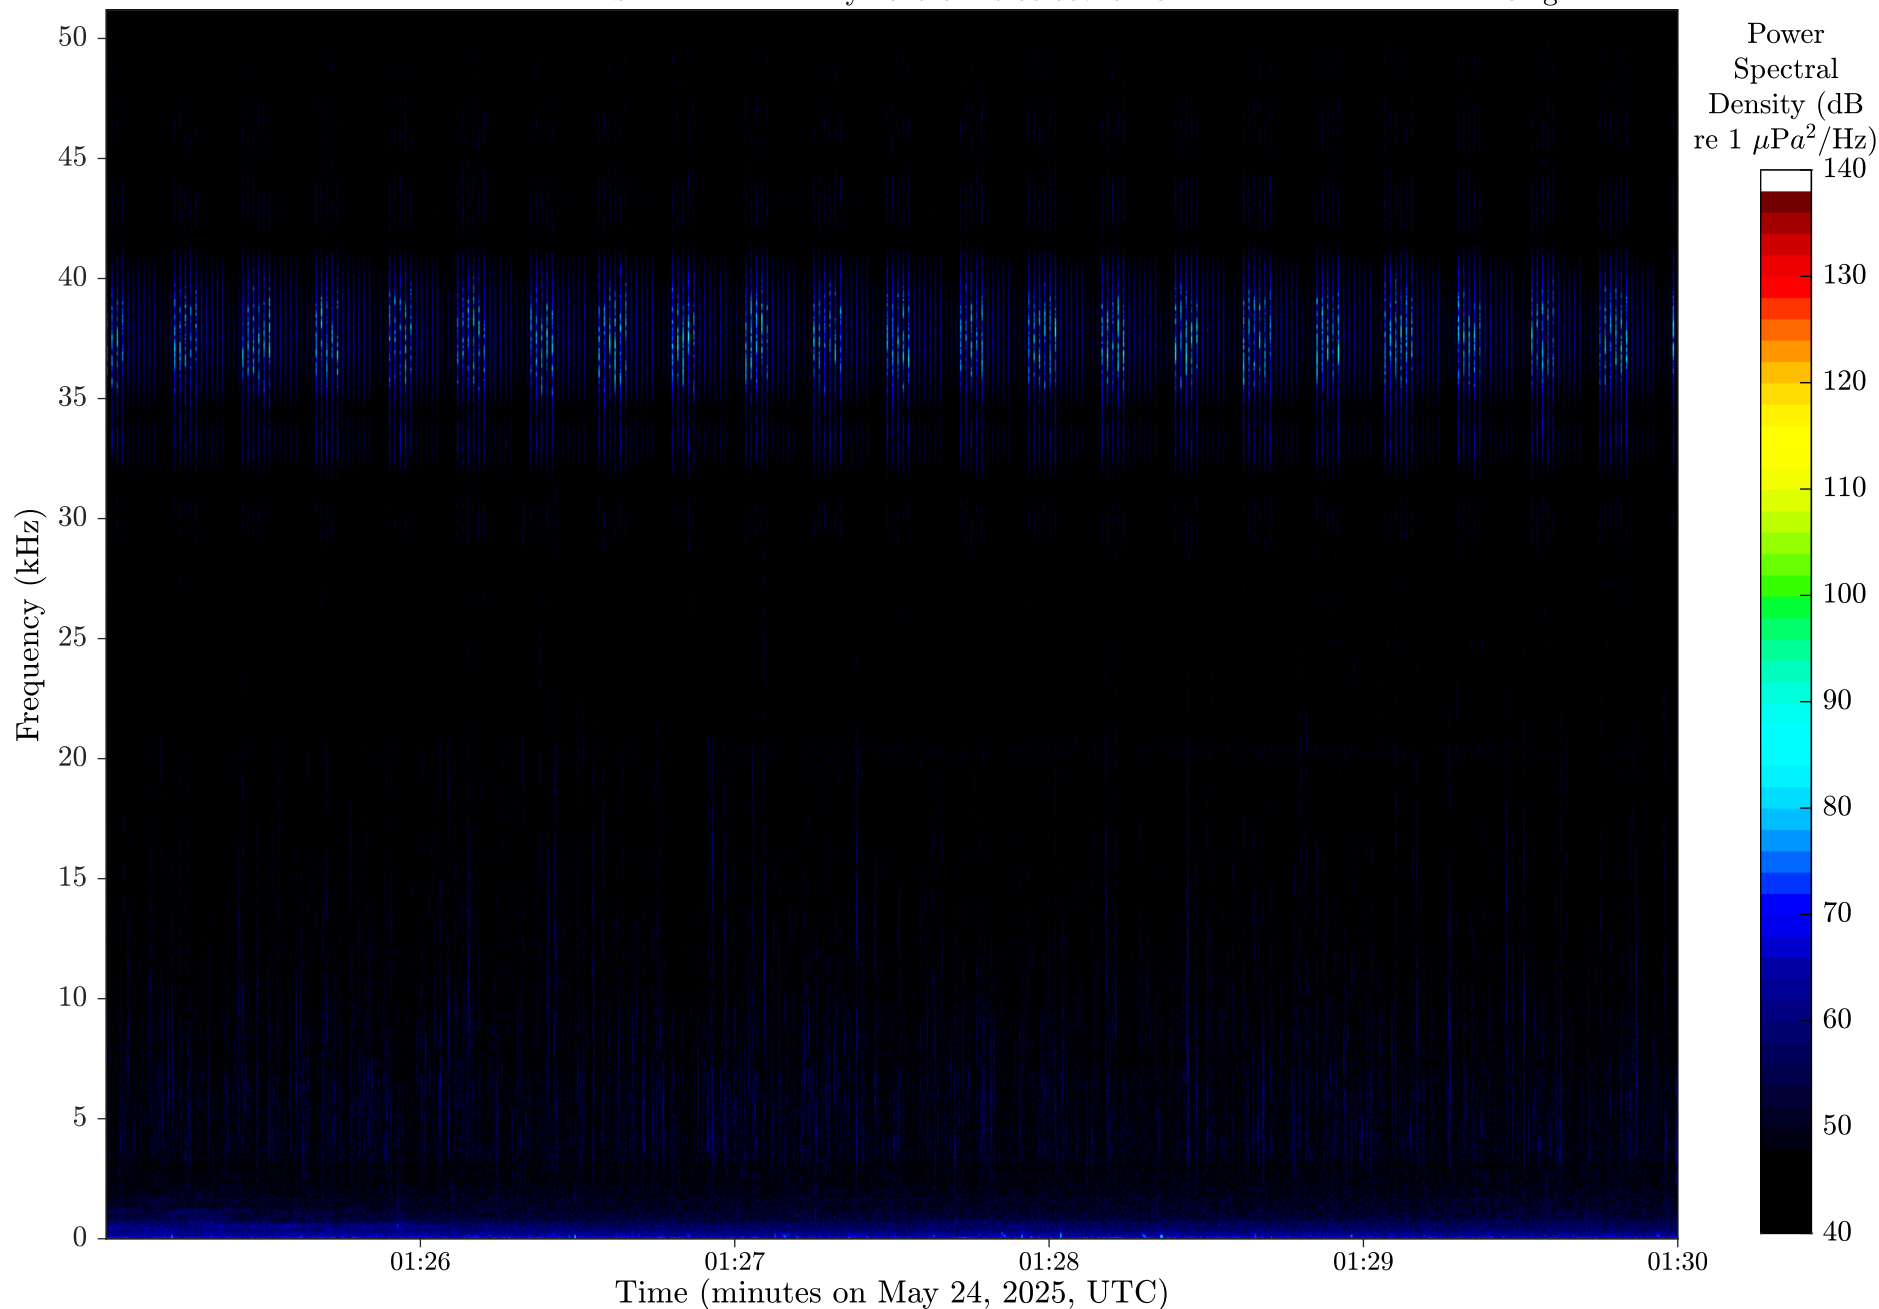

Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:14:17 UTC

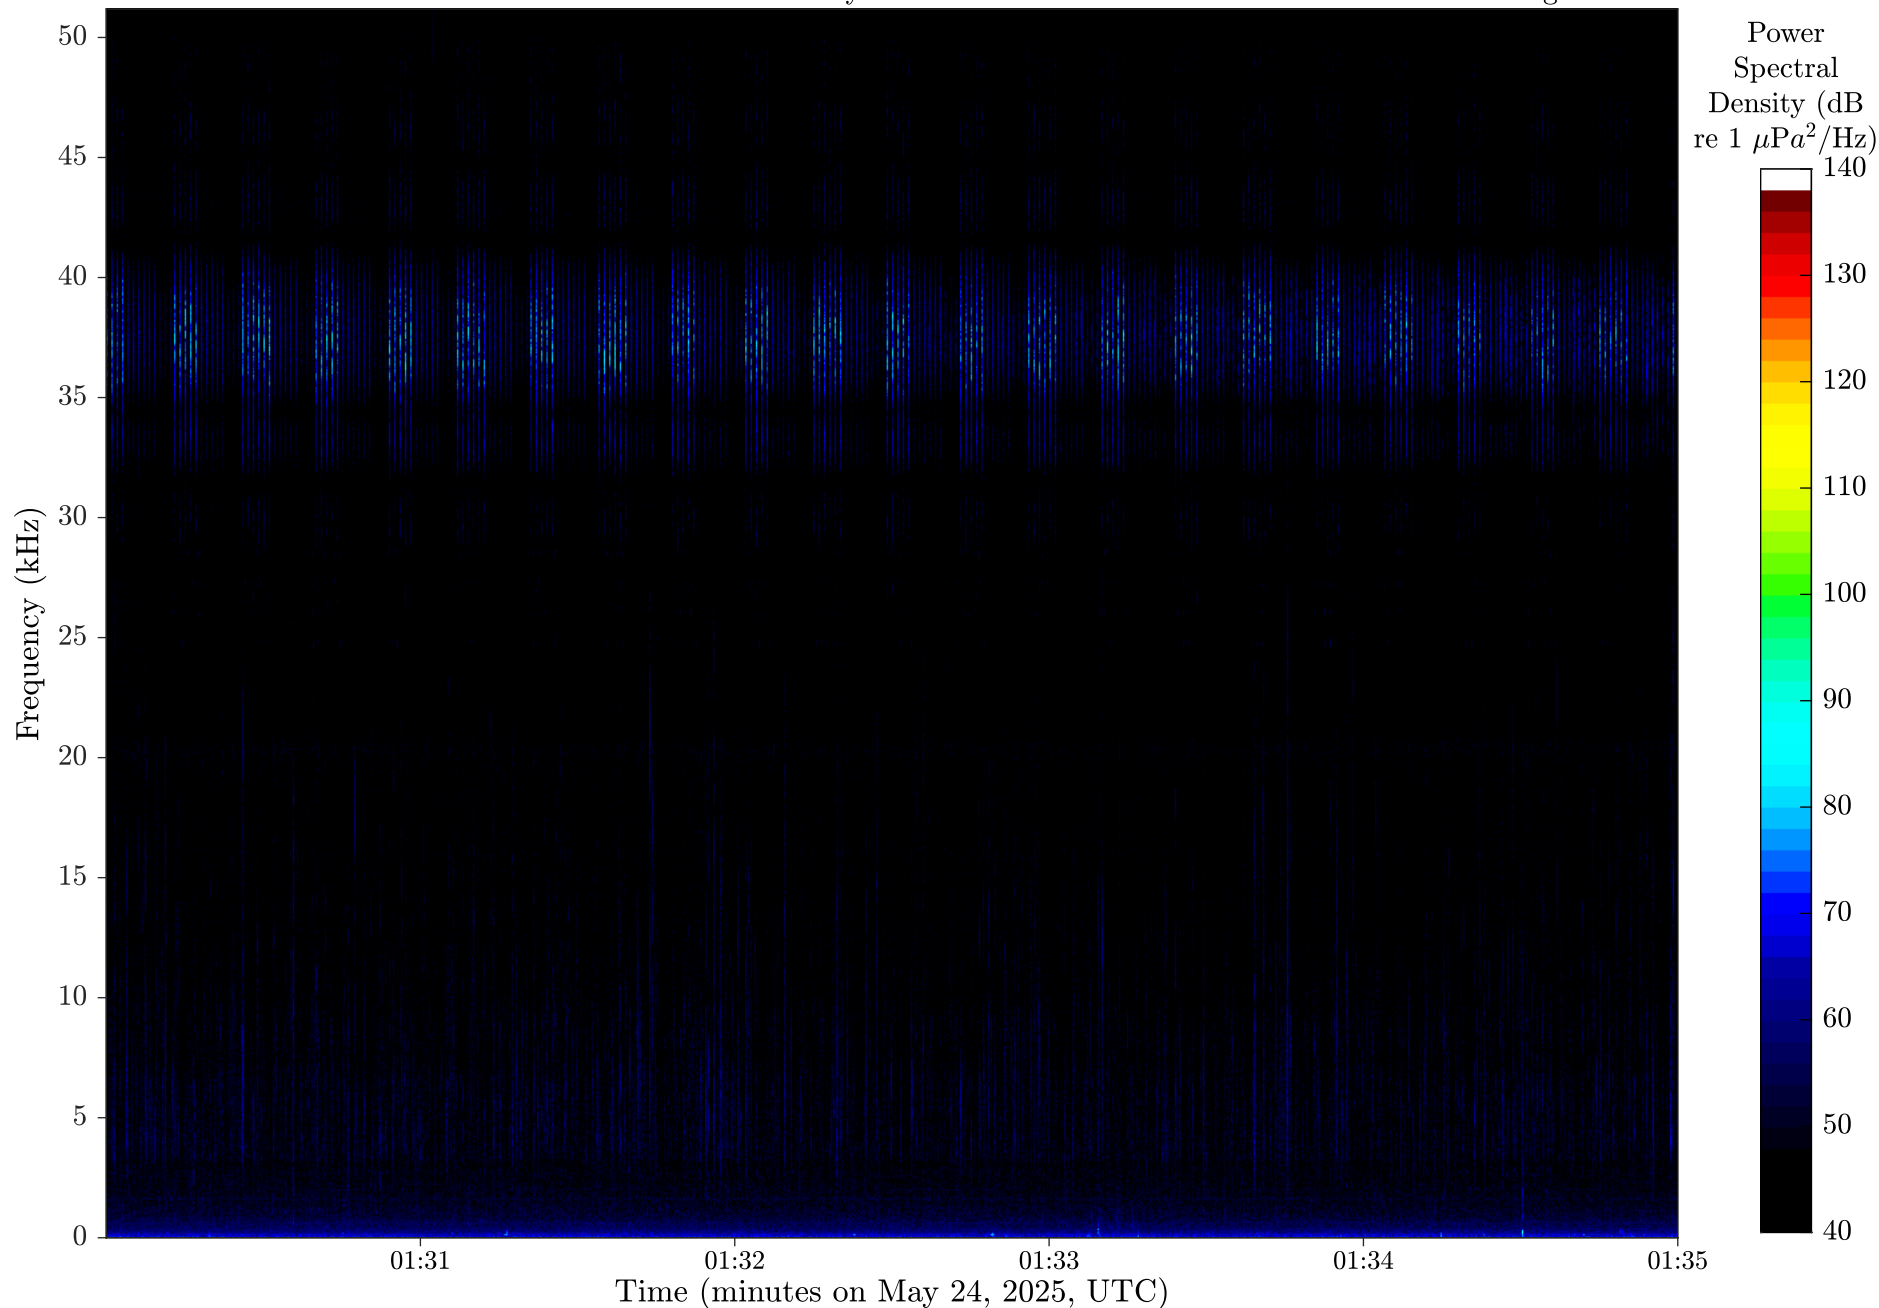

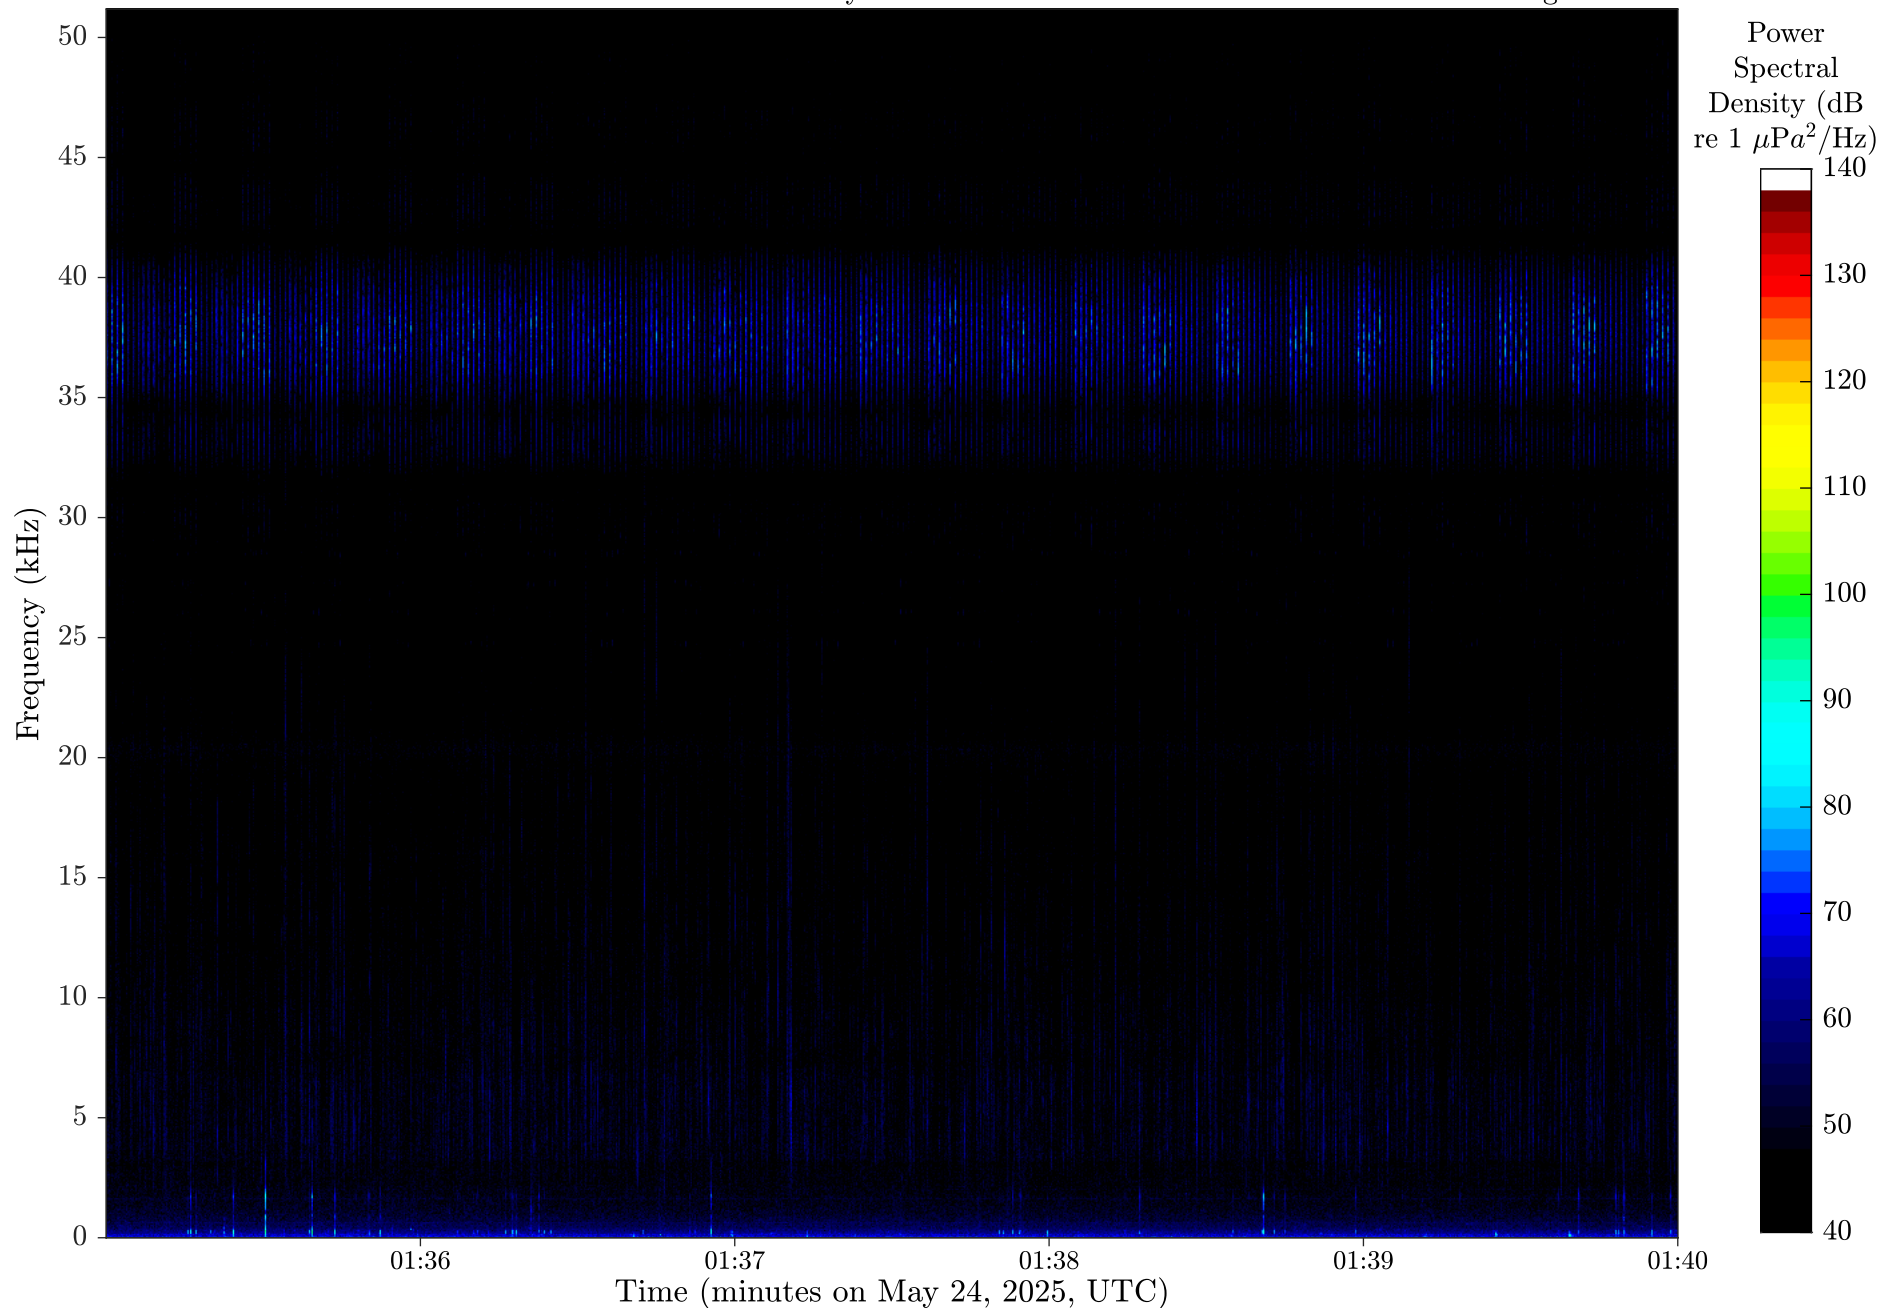


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:14:31 UTC

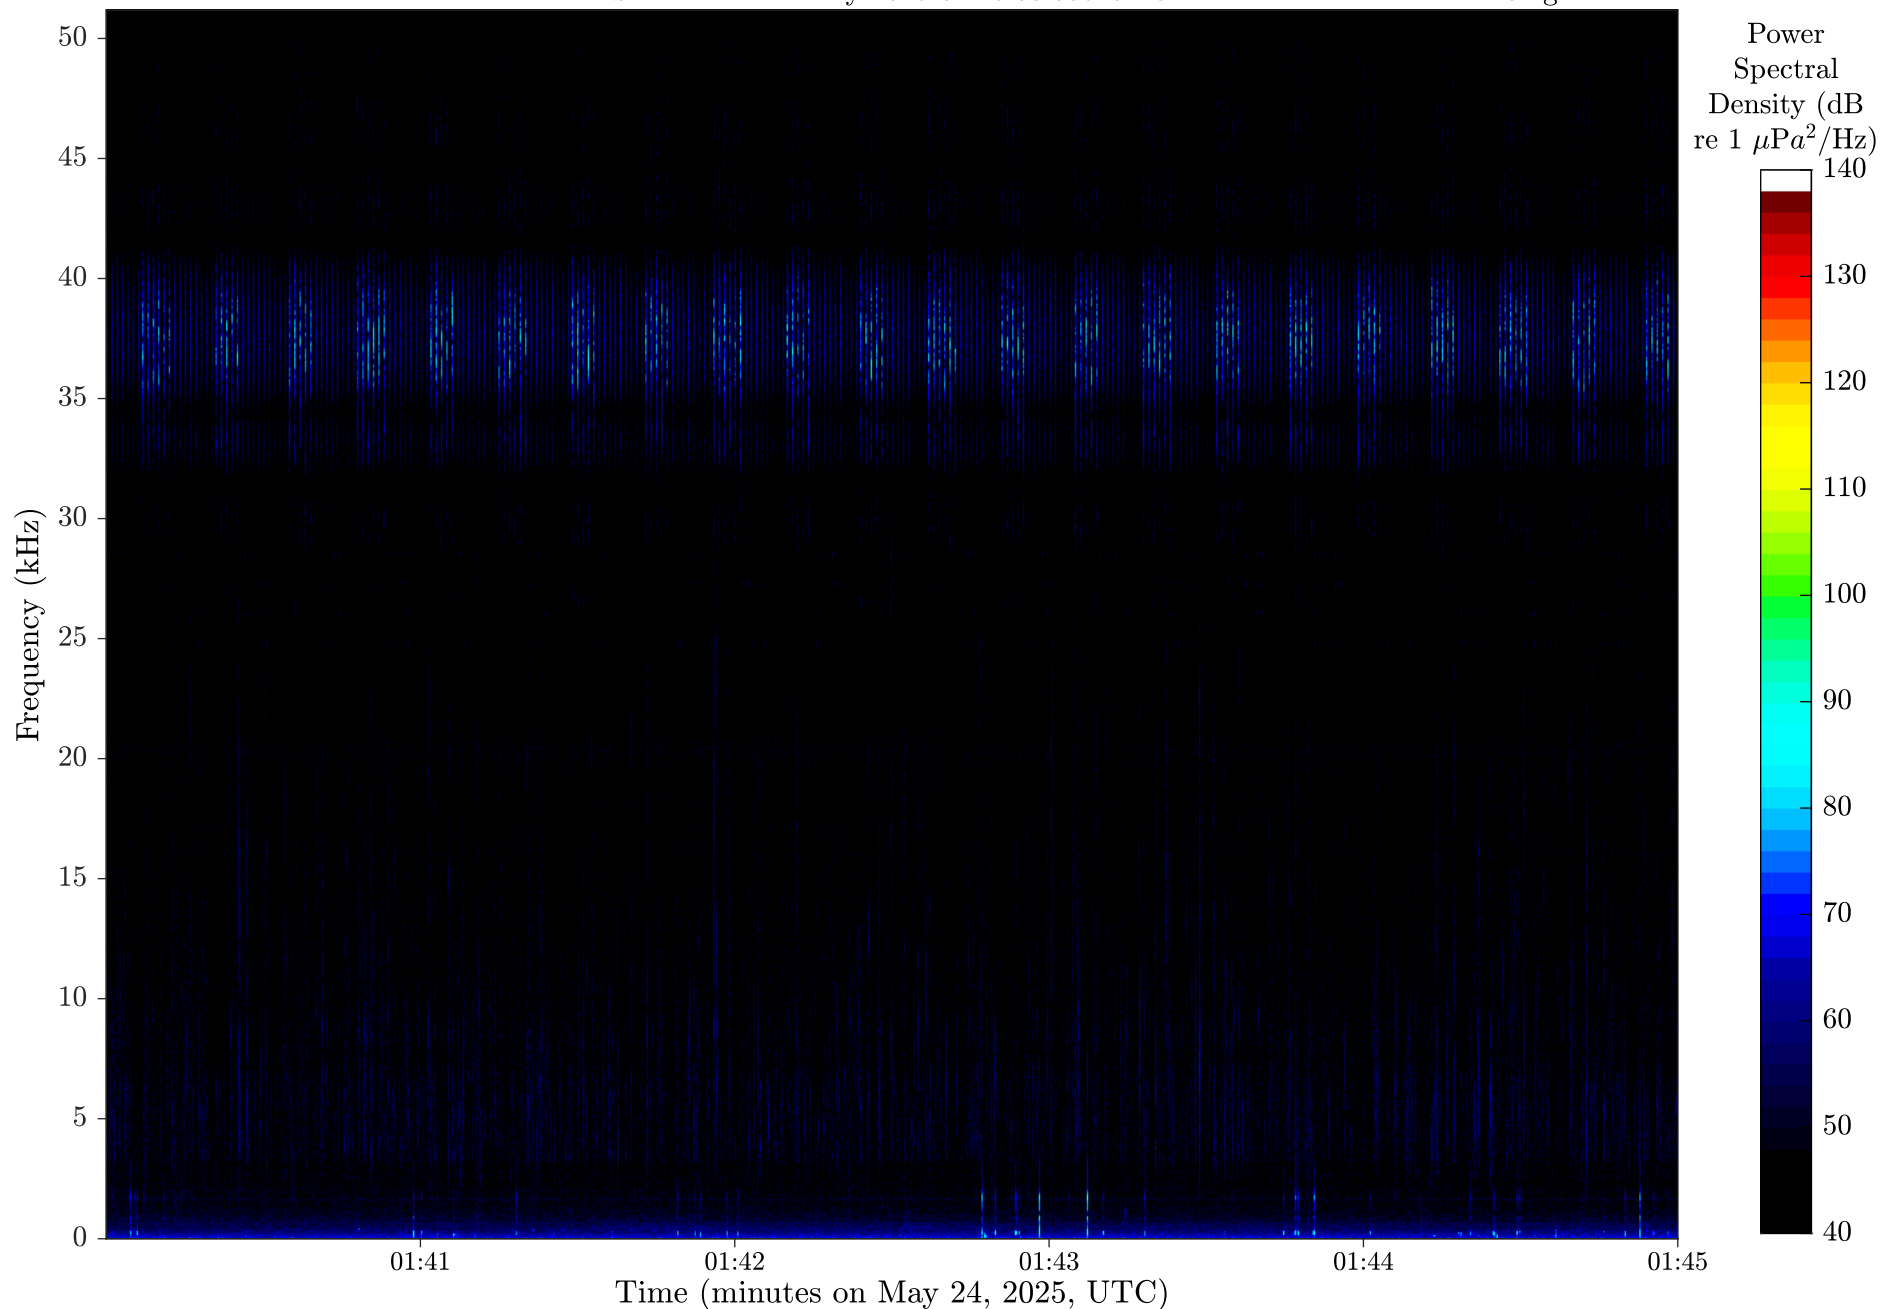


Comments: 34.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:14:38 UTC

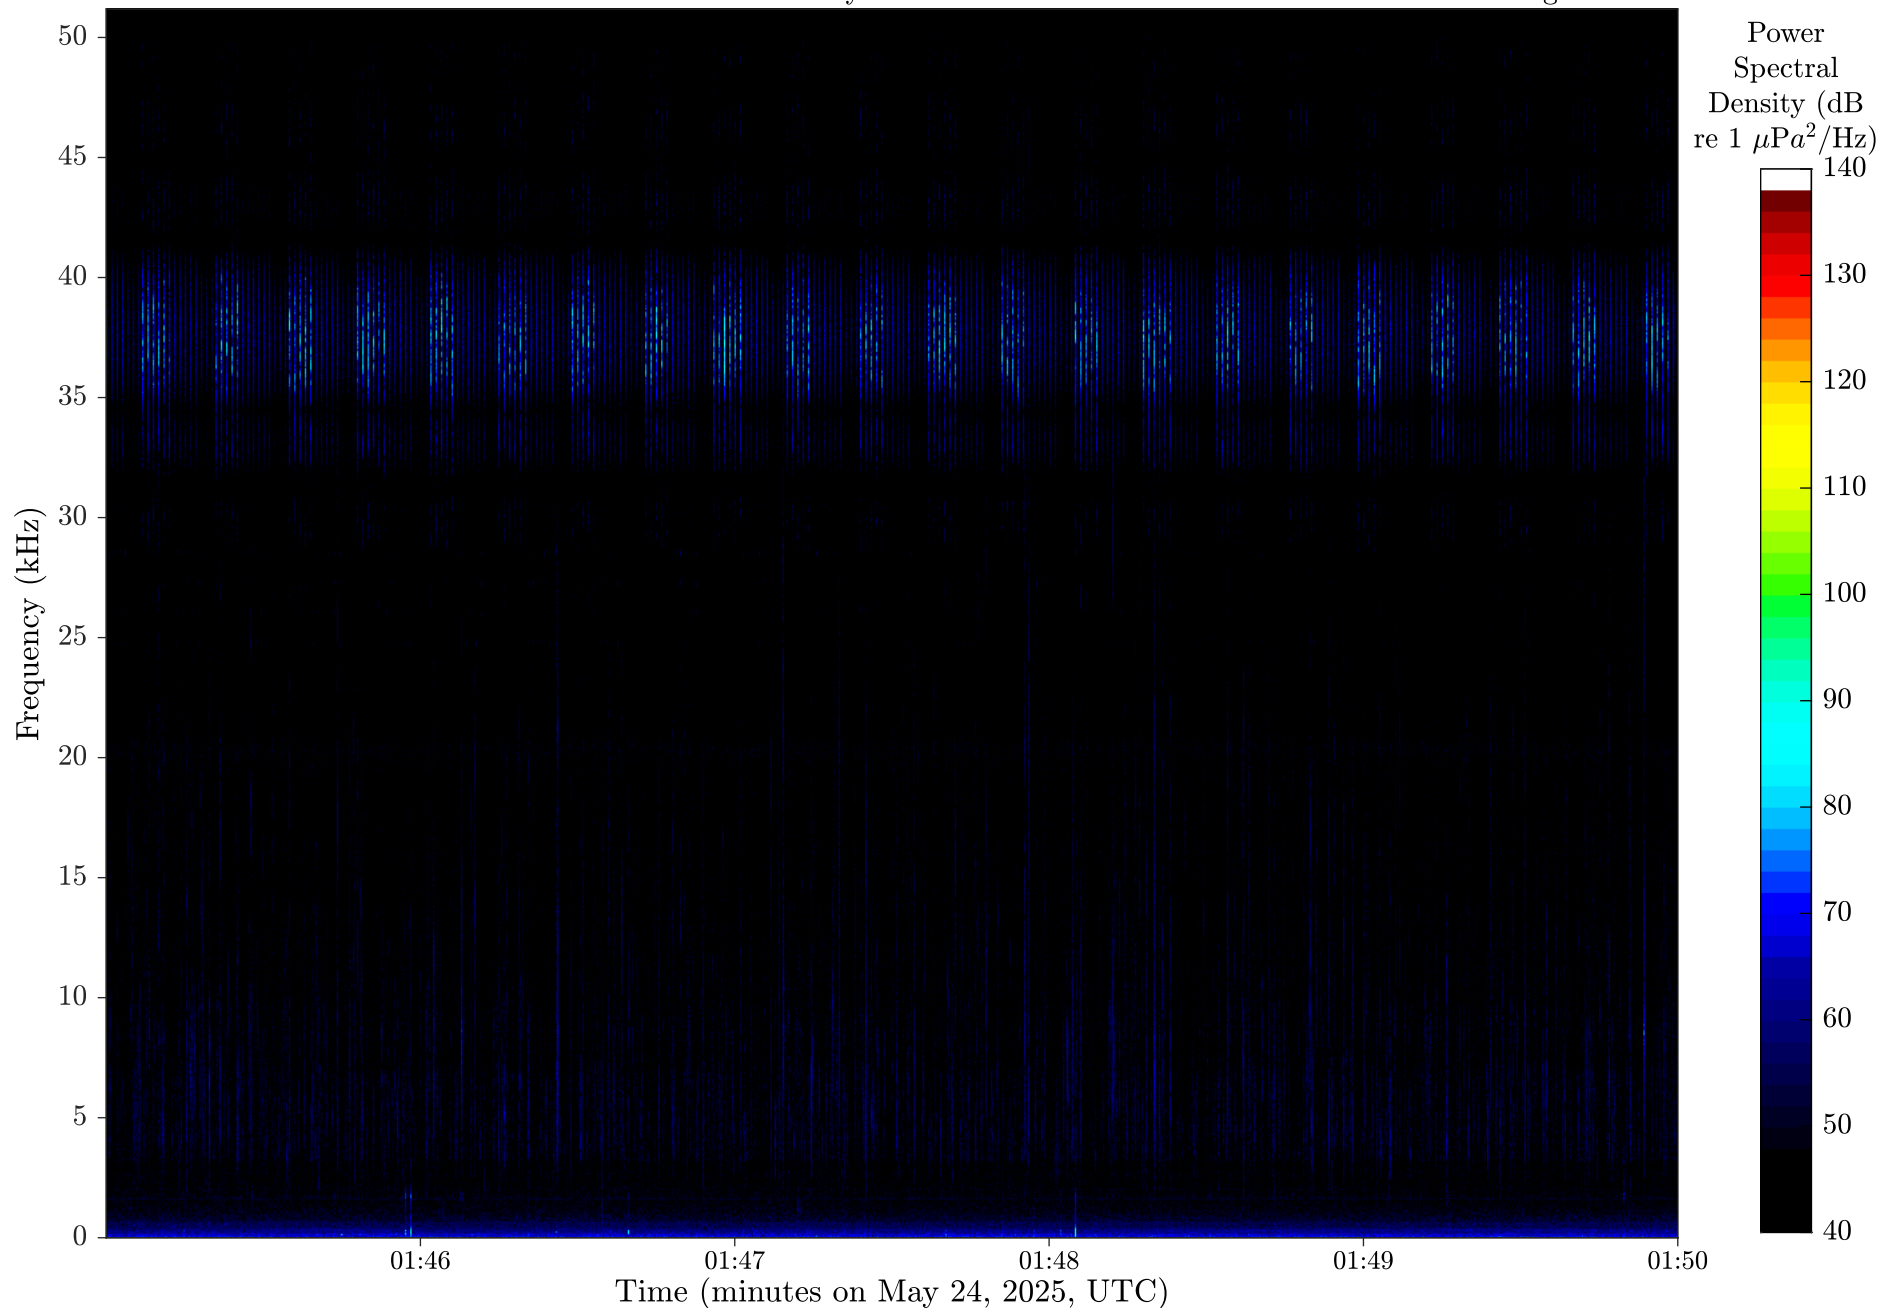


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:14:45 UTC

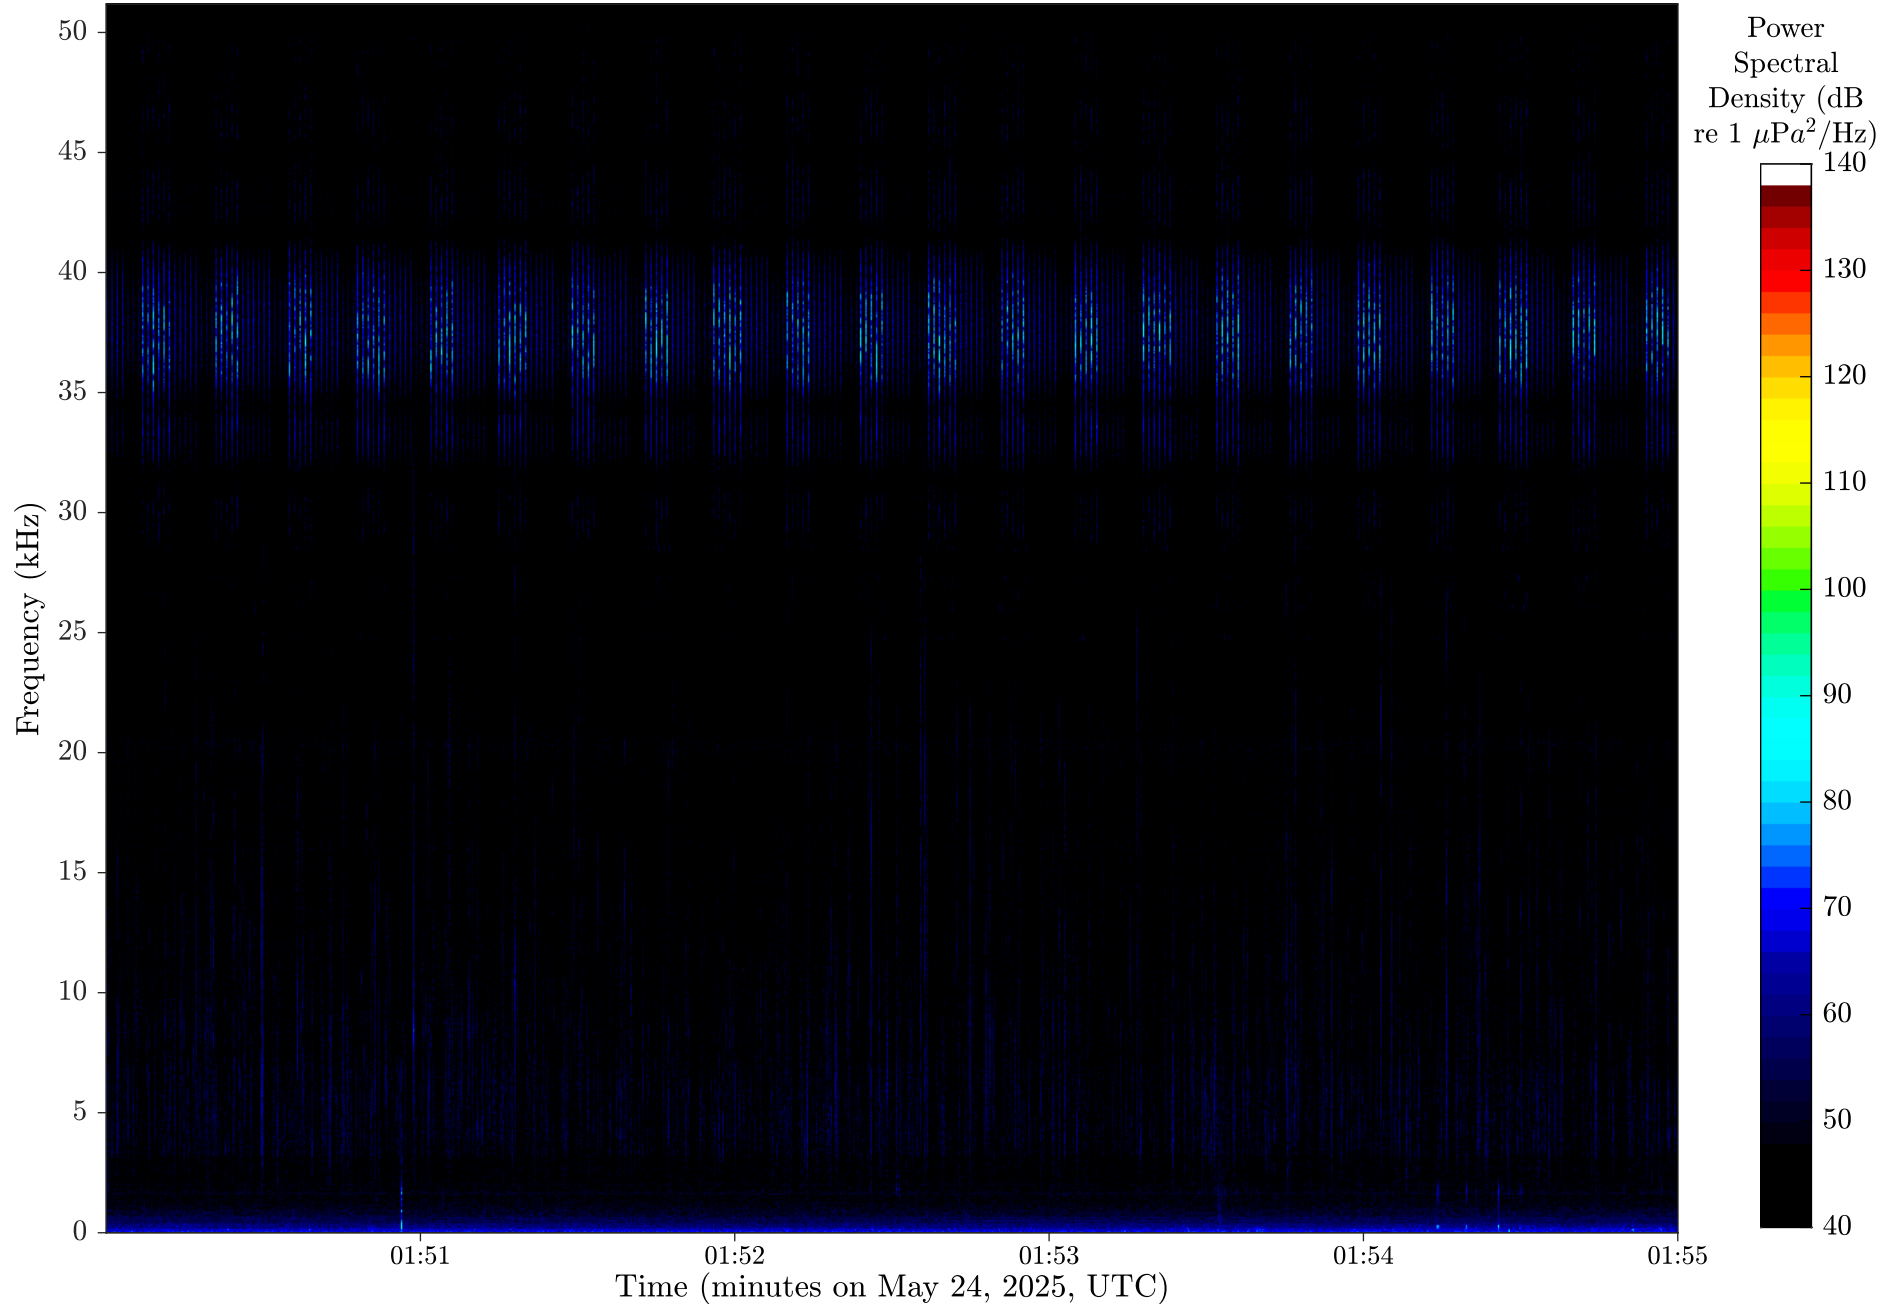


Comments: 36.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:14:52 UTC

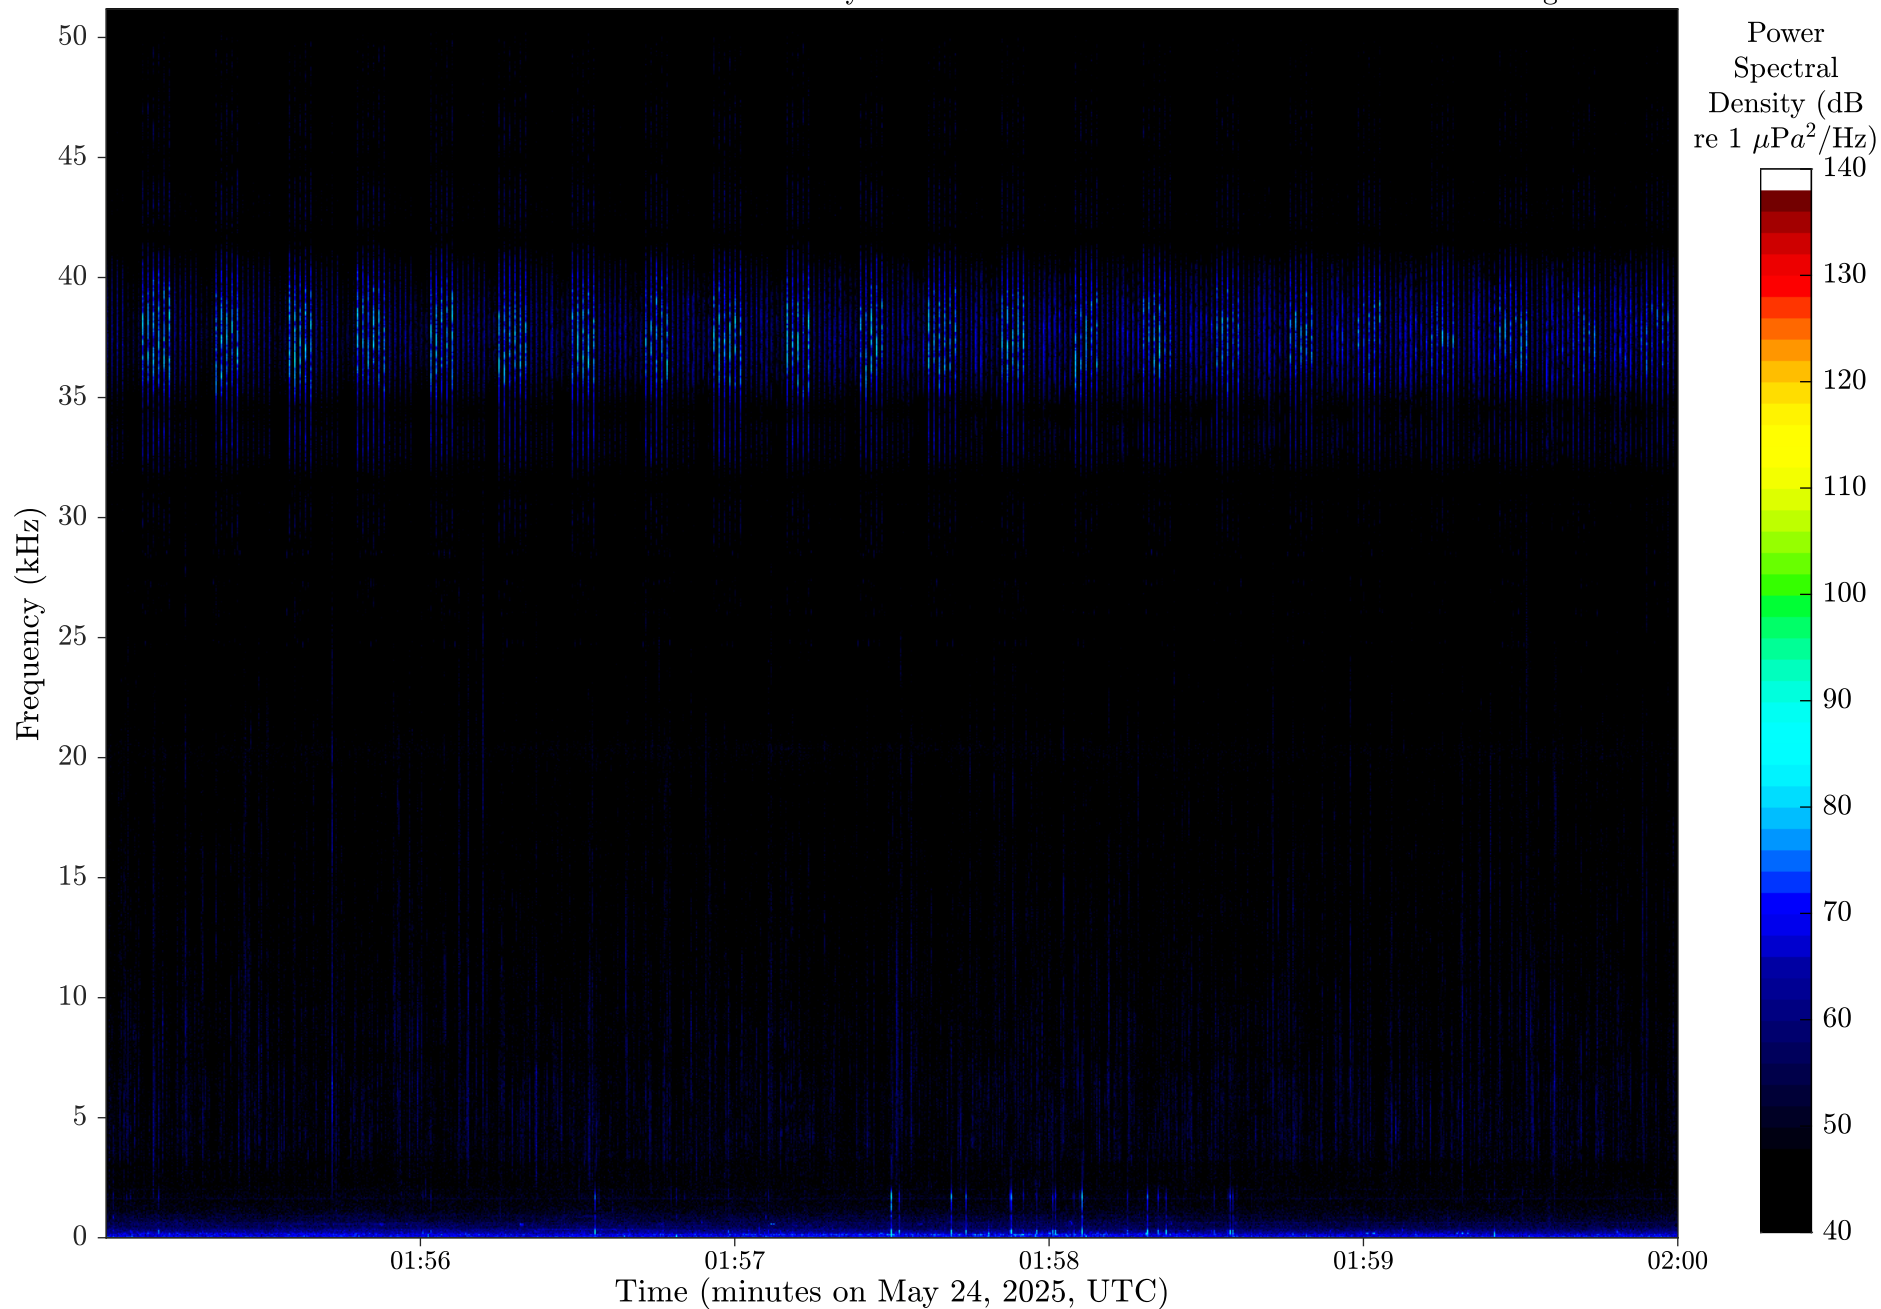

Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:14:59 UTC

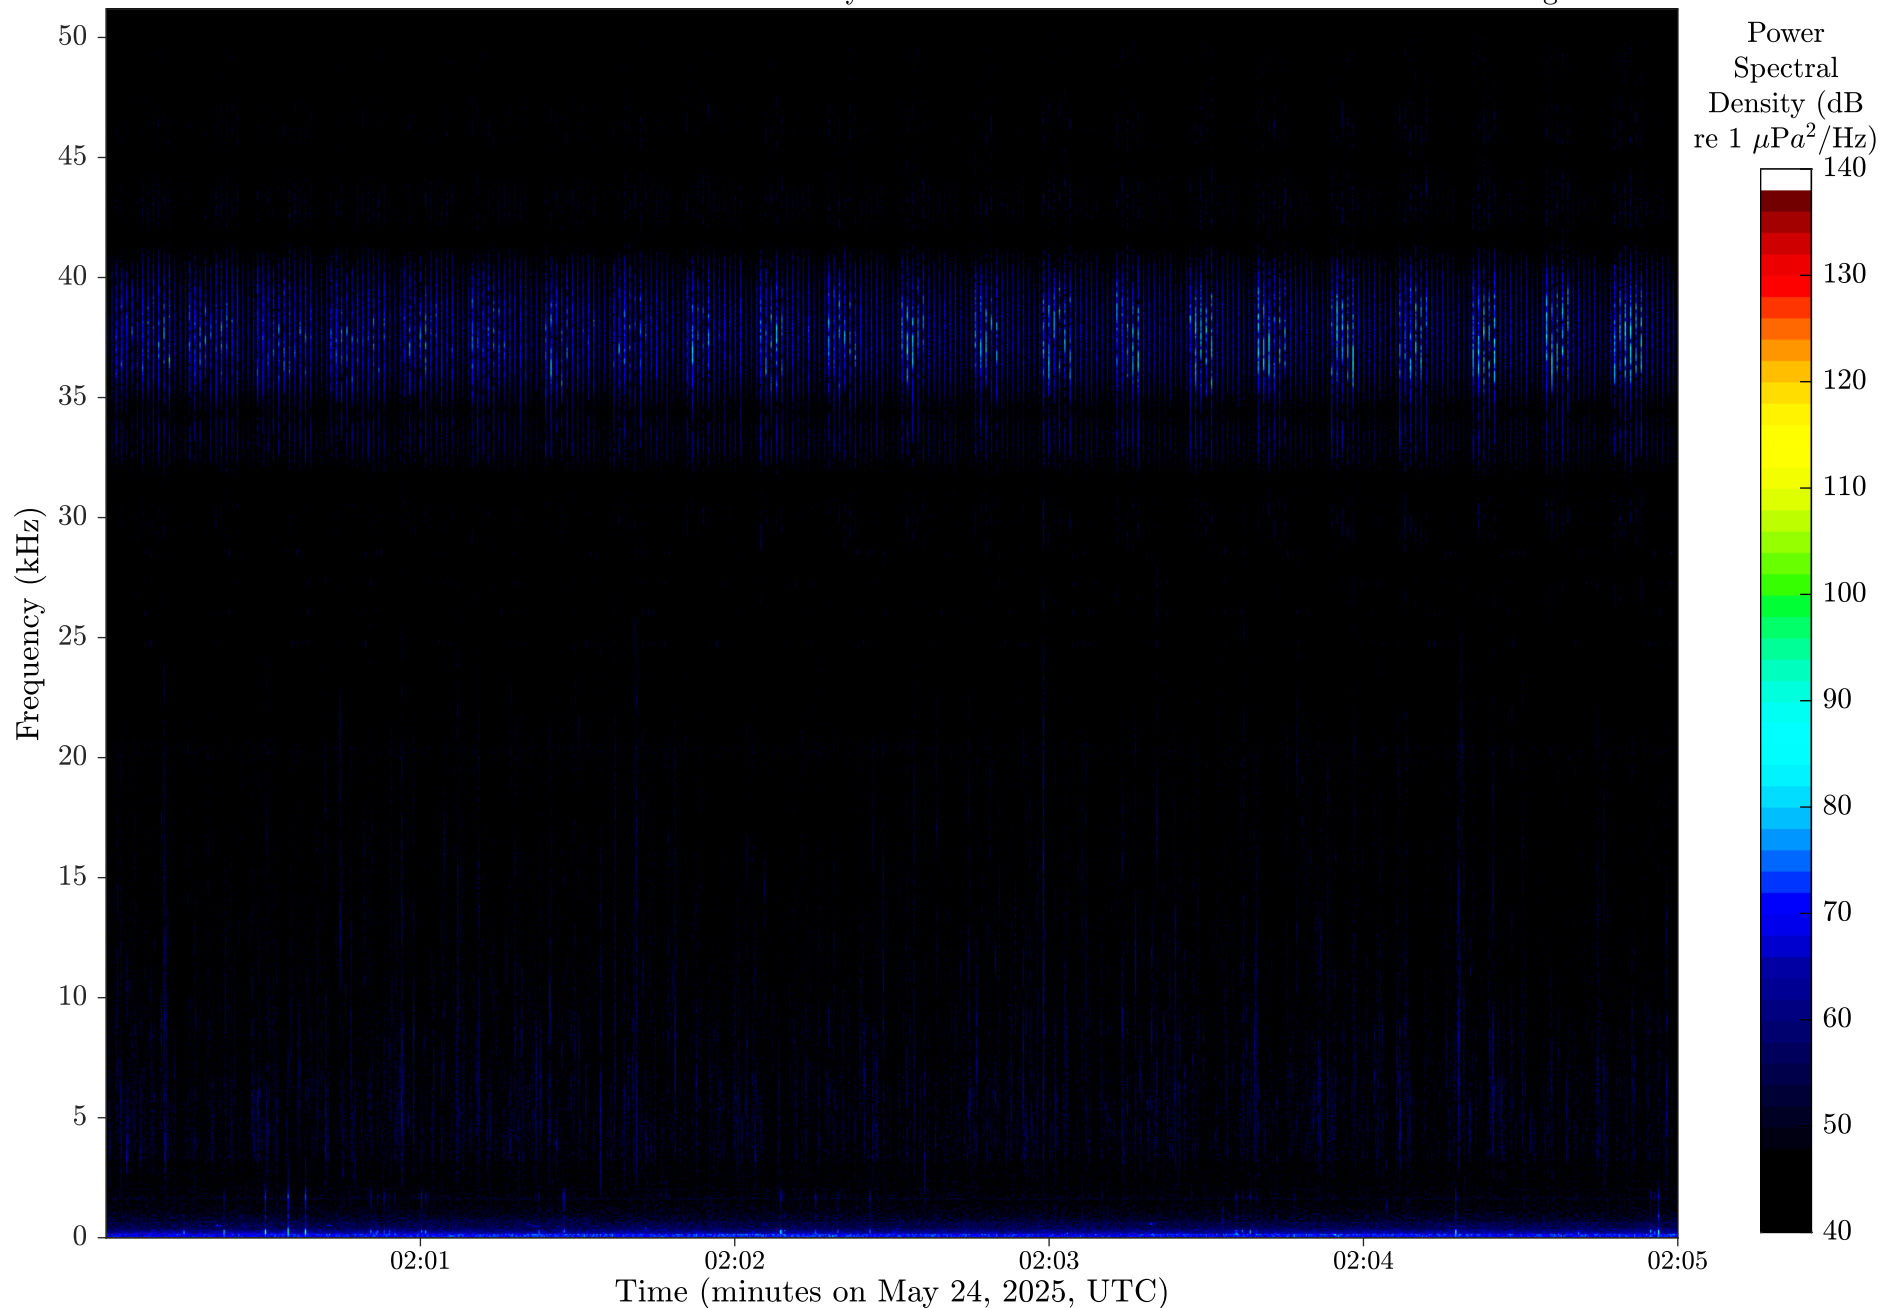

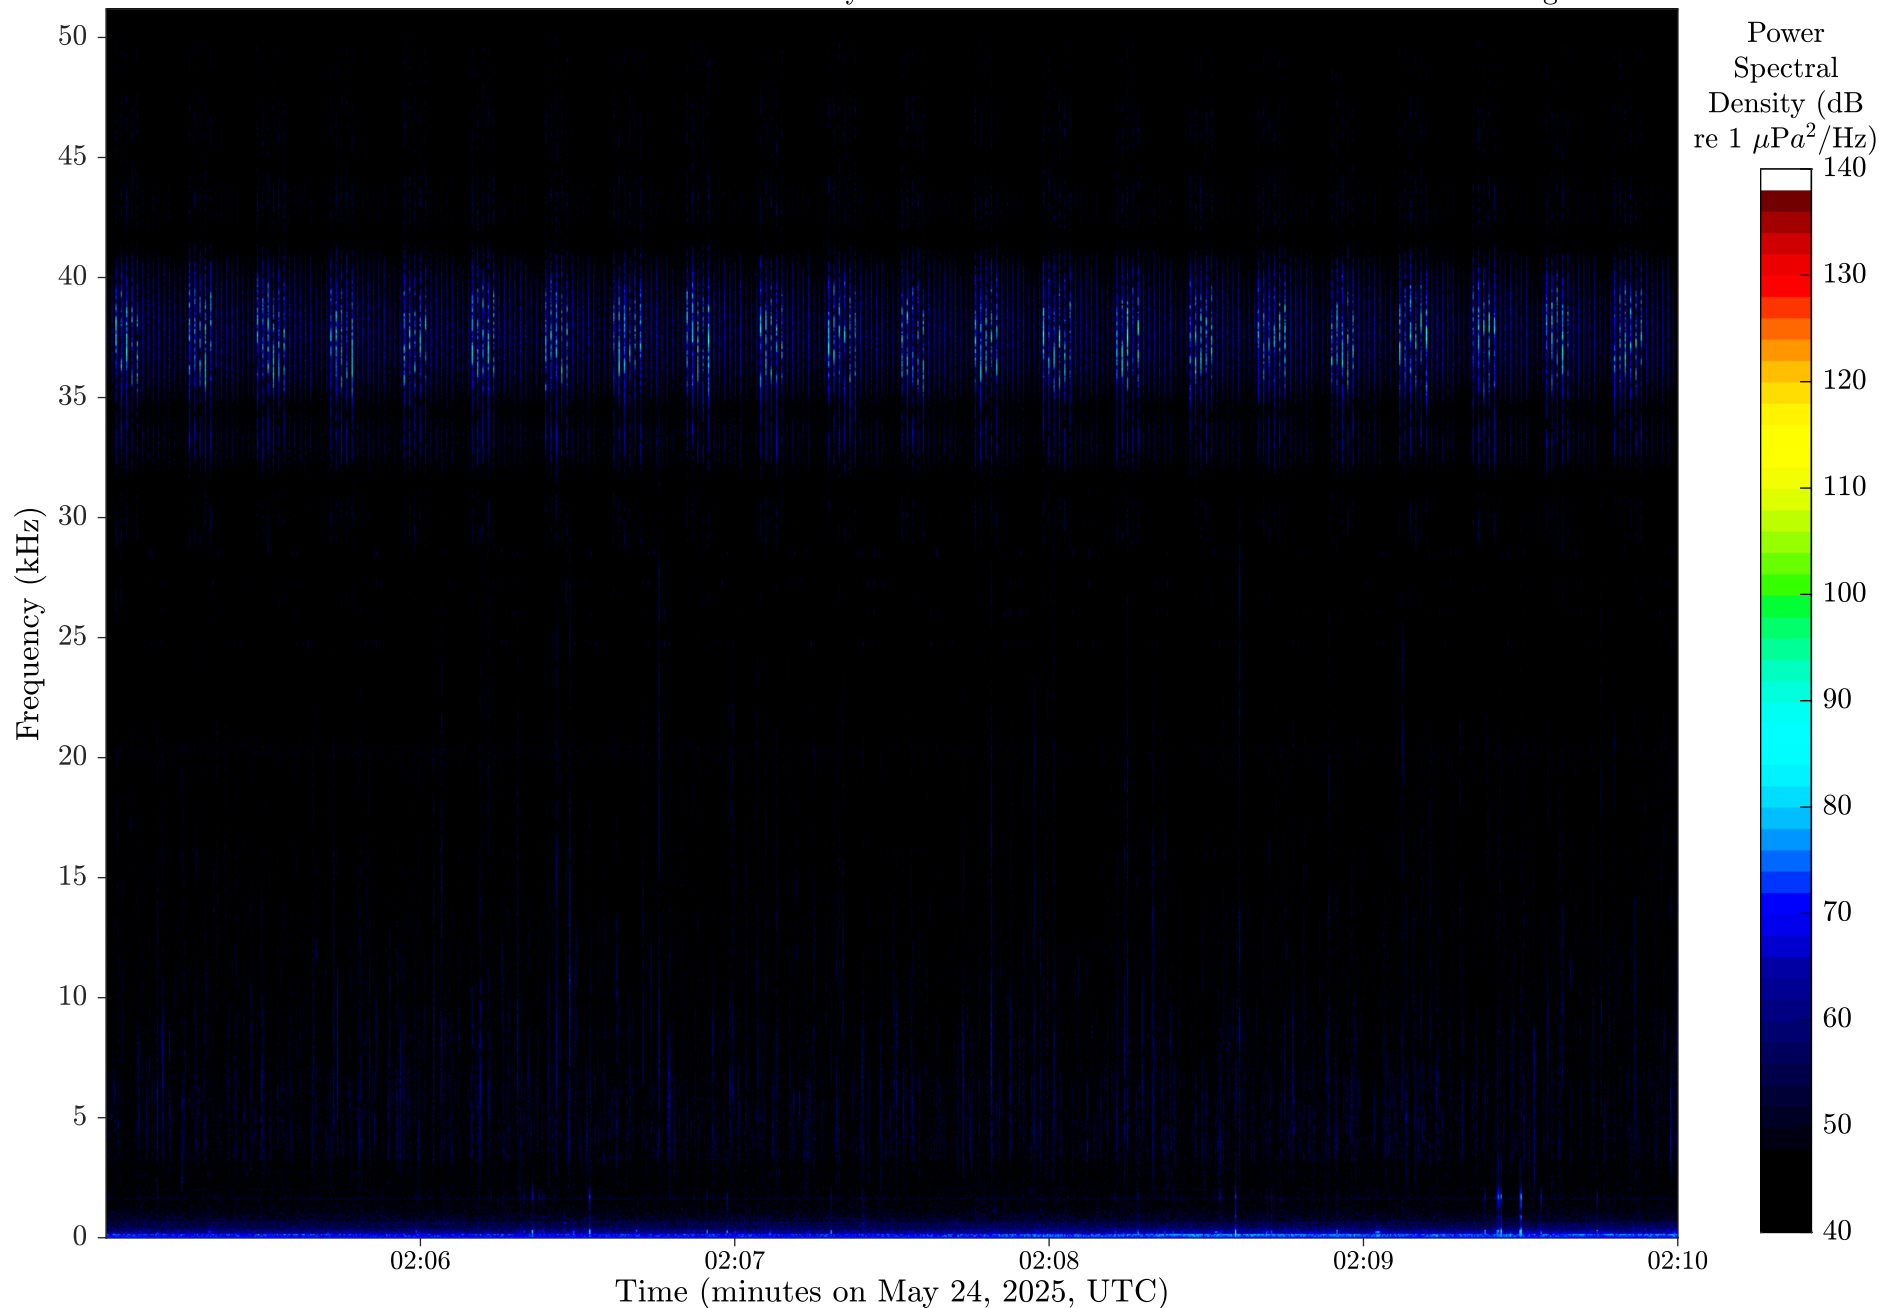


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:15:15 UTC

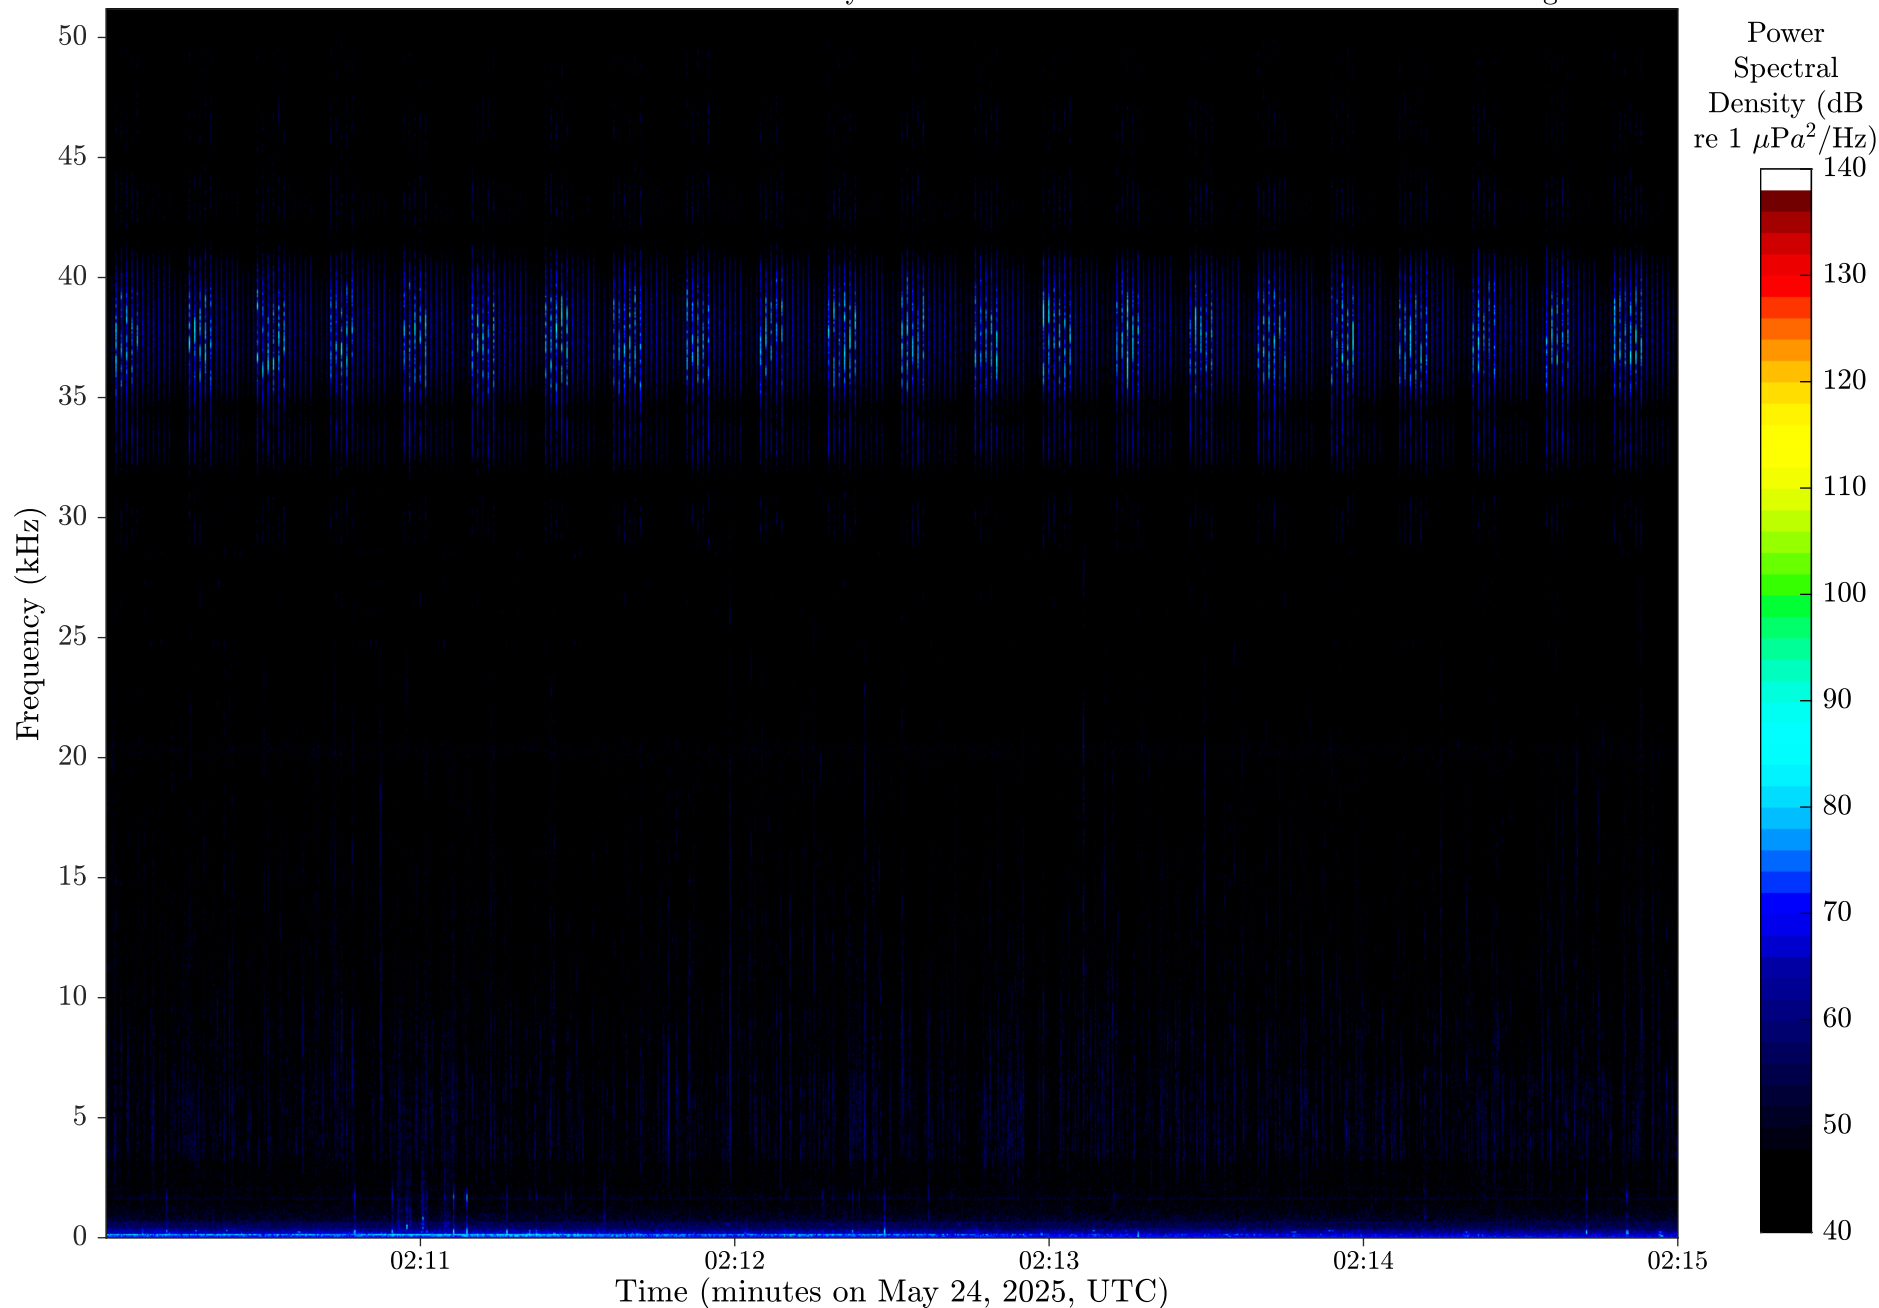


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:15:22 UTC

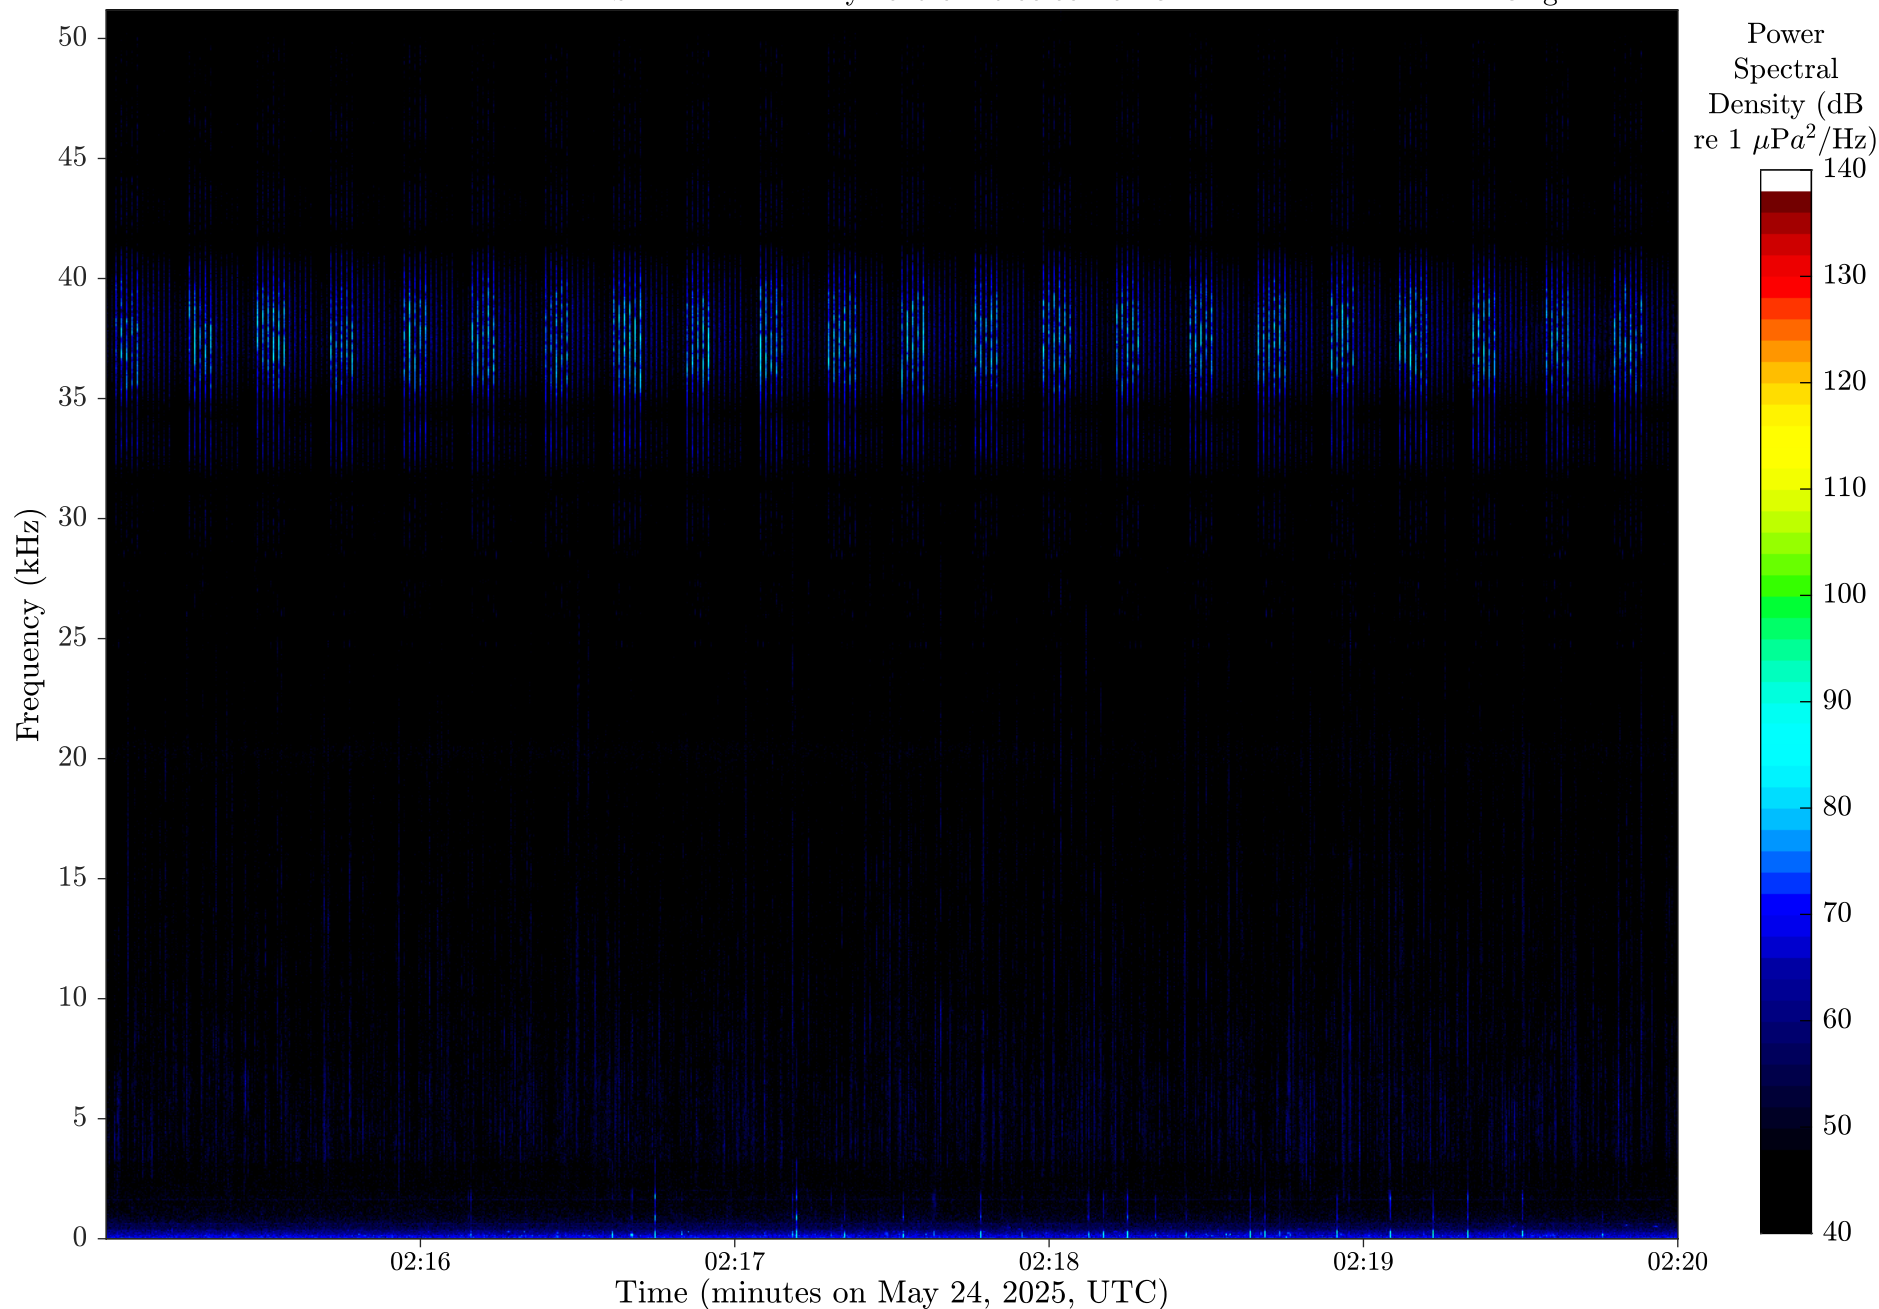


Comments: 35.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:15:30 UTC

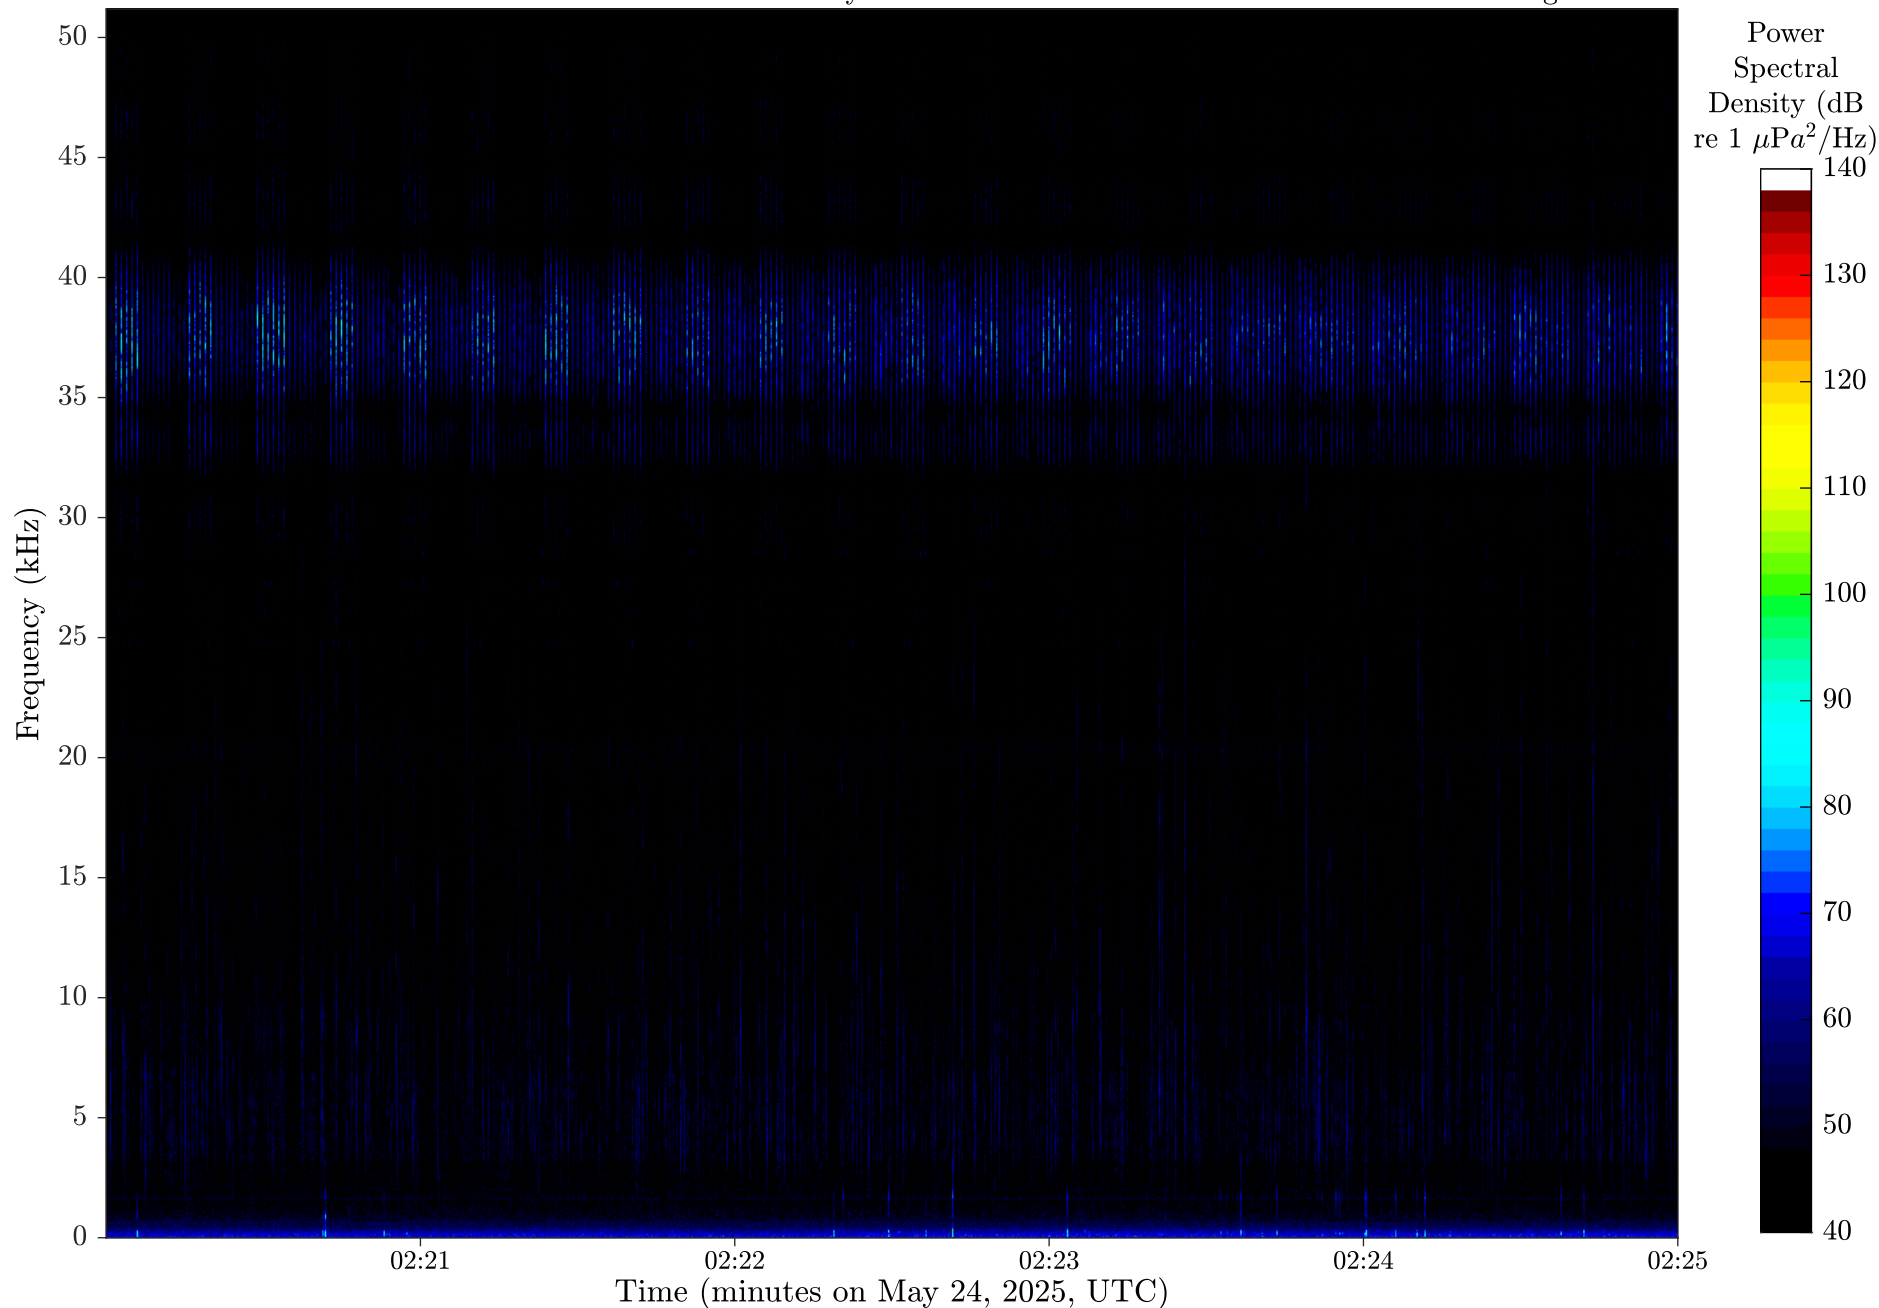


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:15:38 UTC

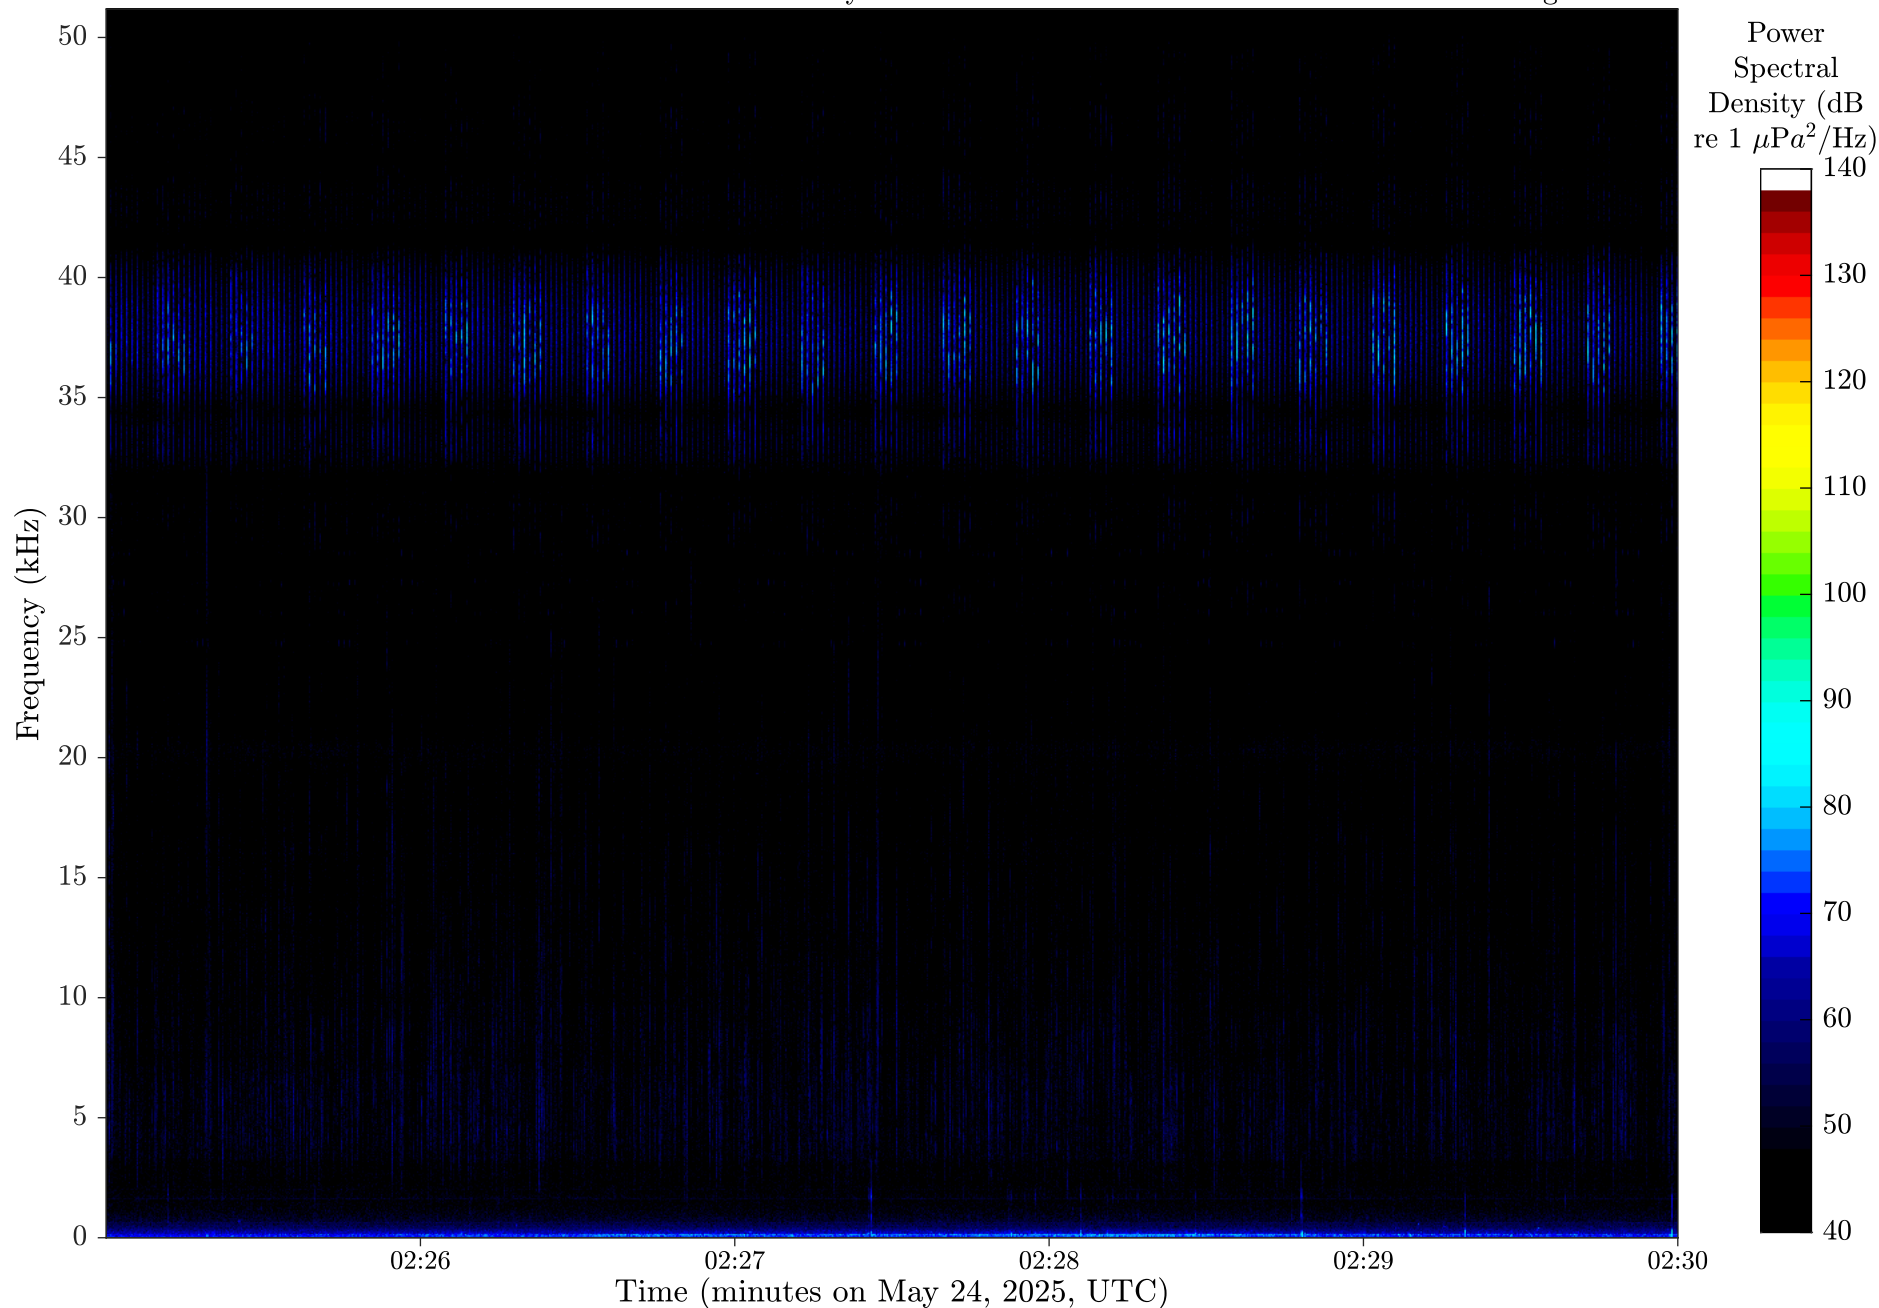


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:15:45 UTC

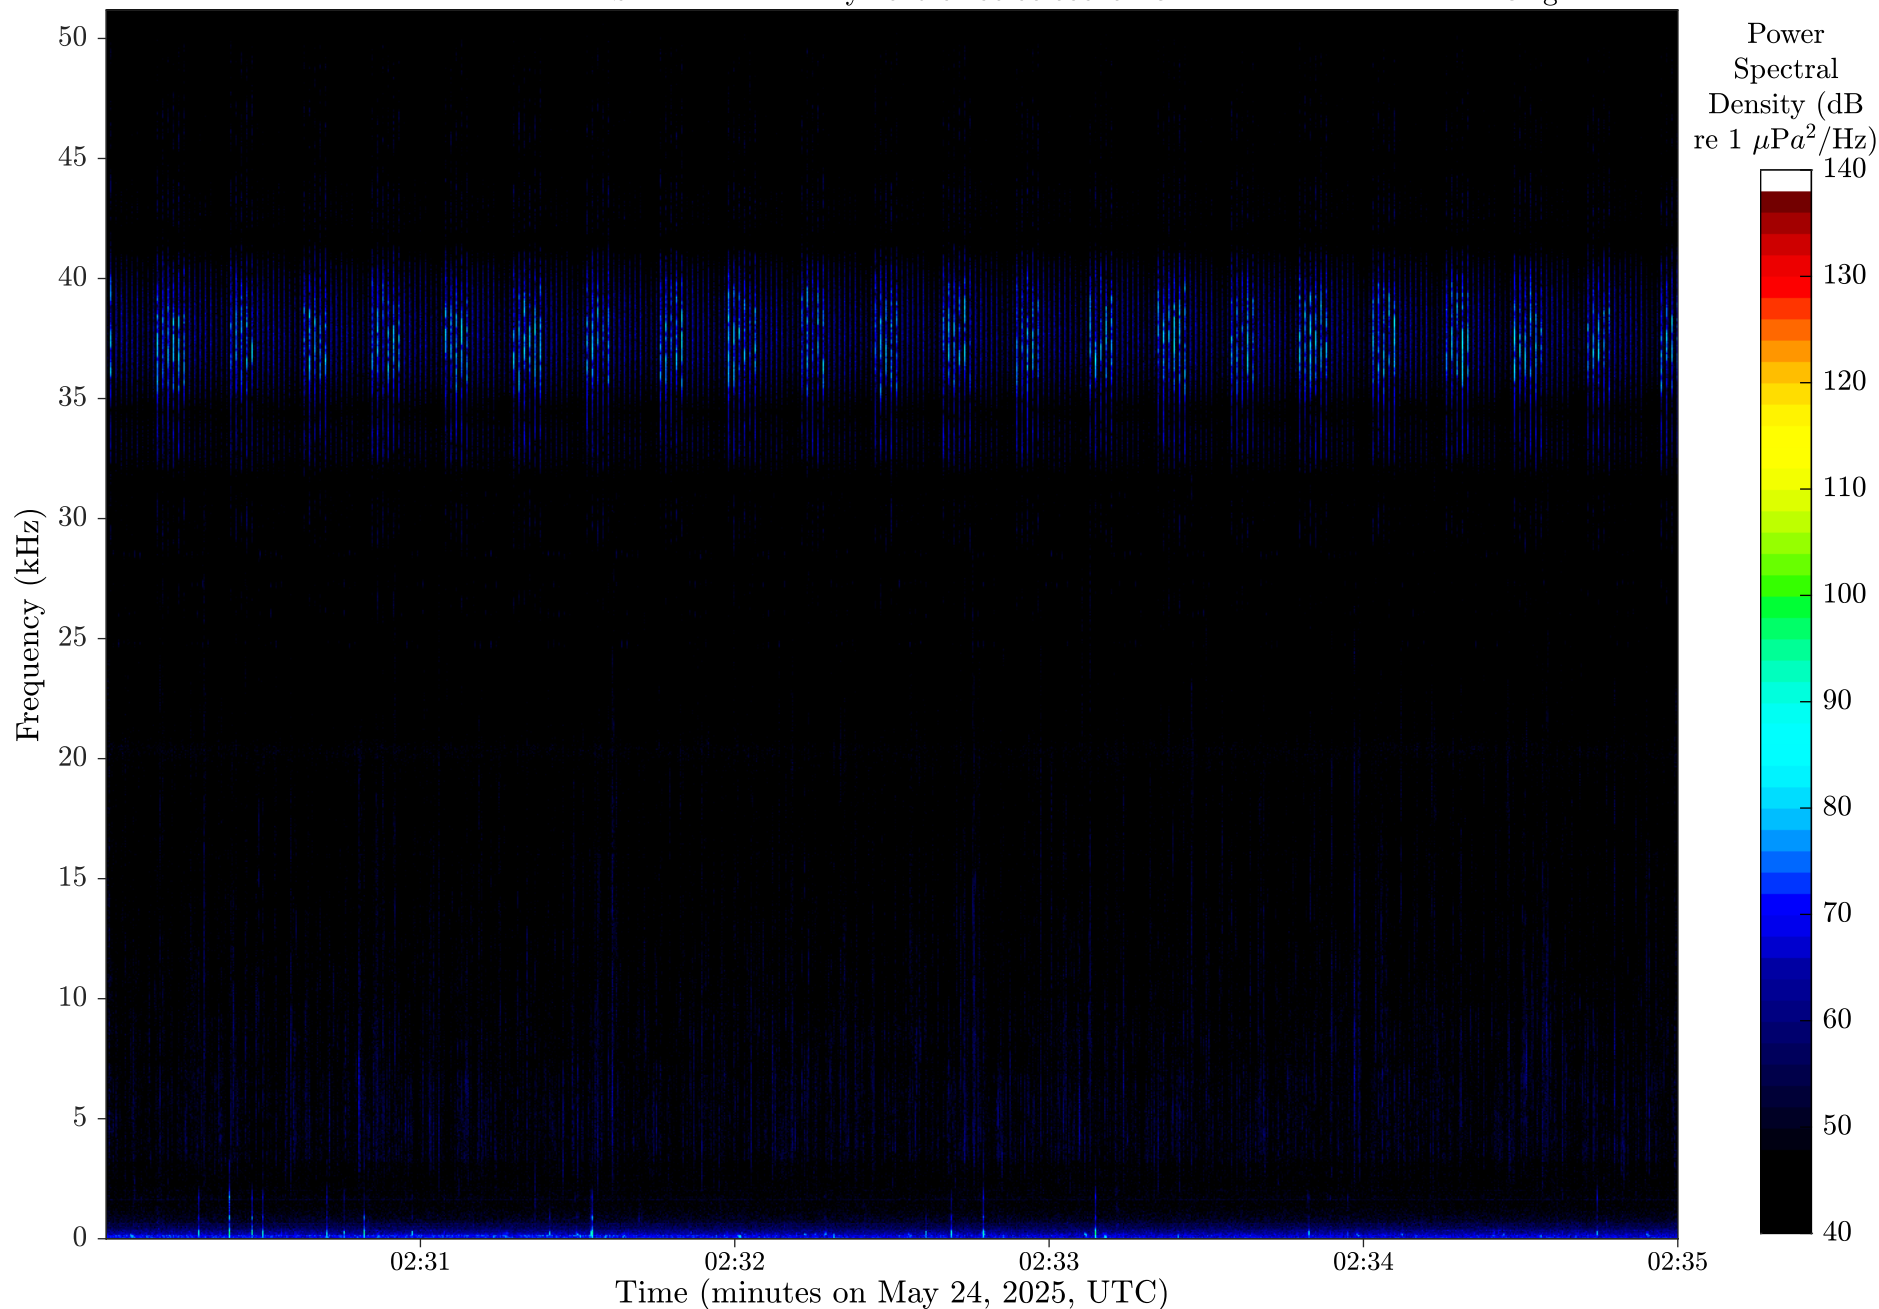


Comments: 35.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:15:52 UTC

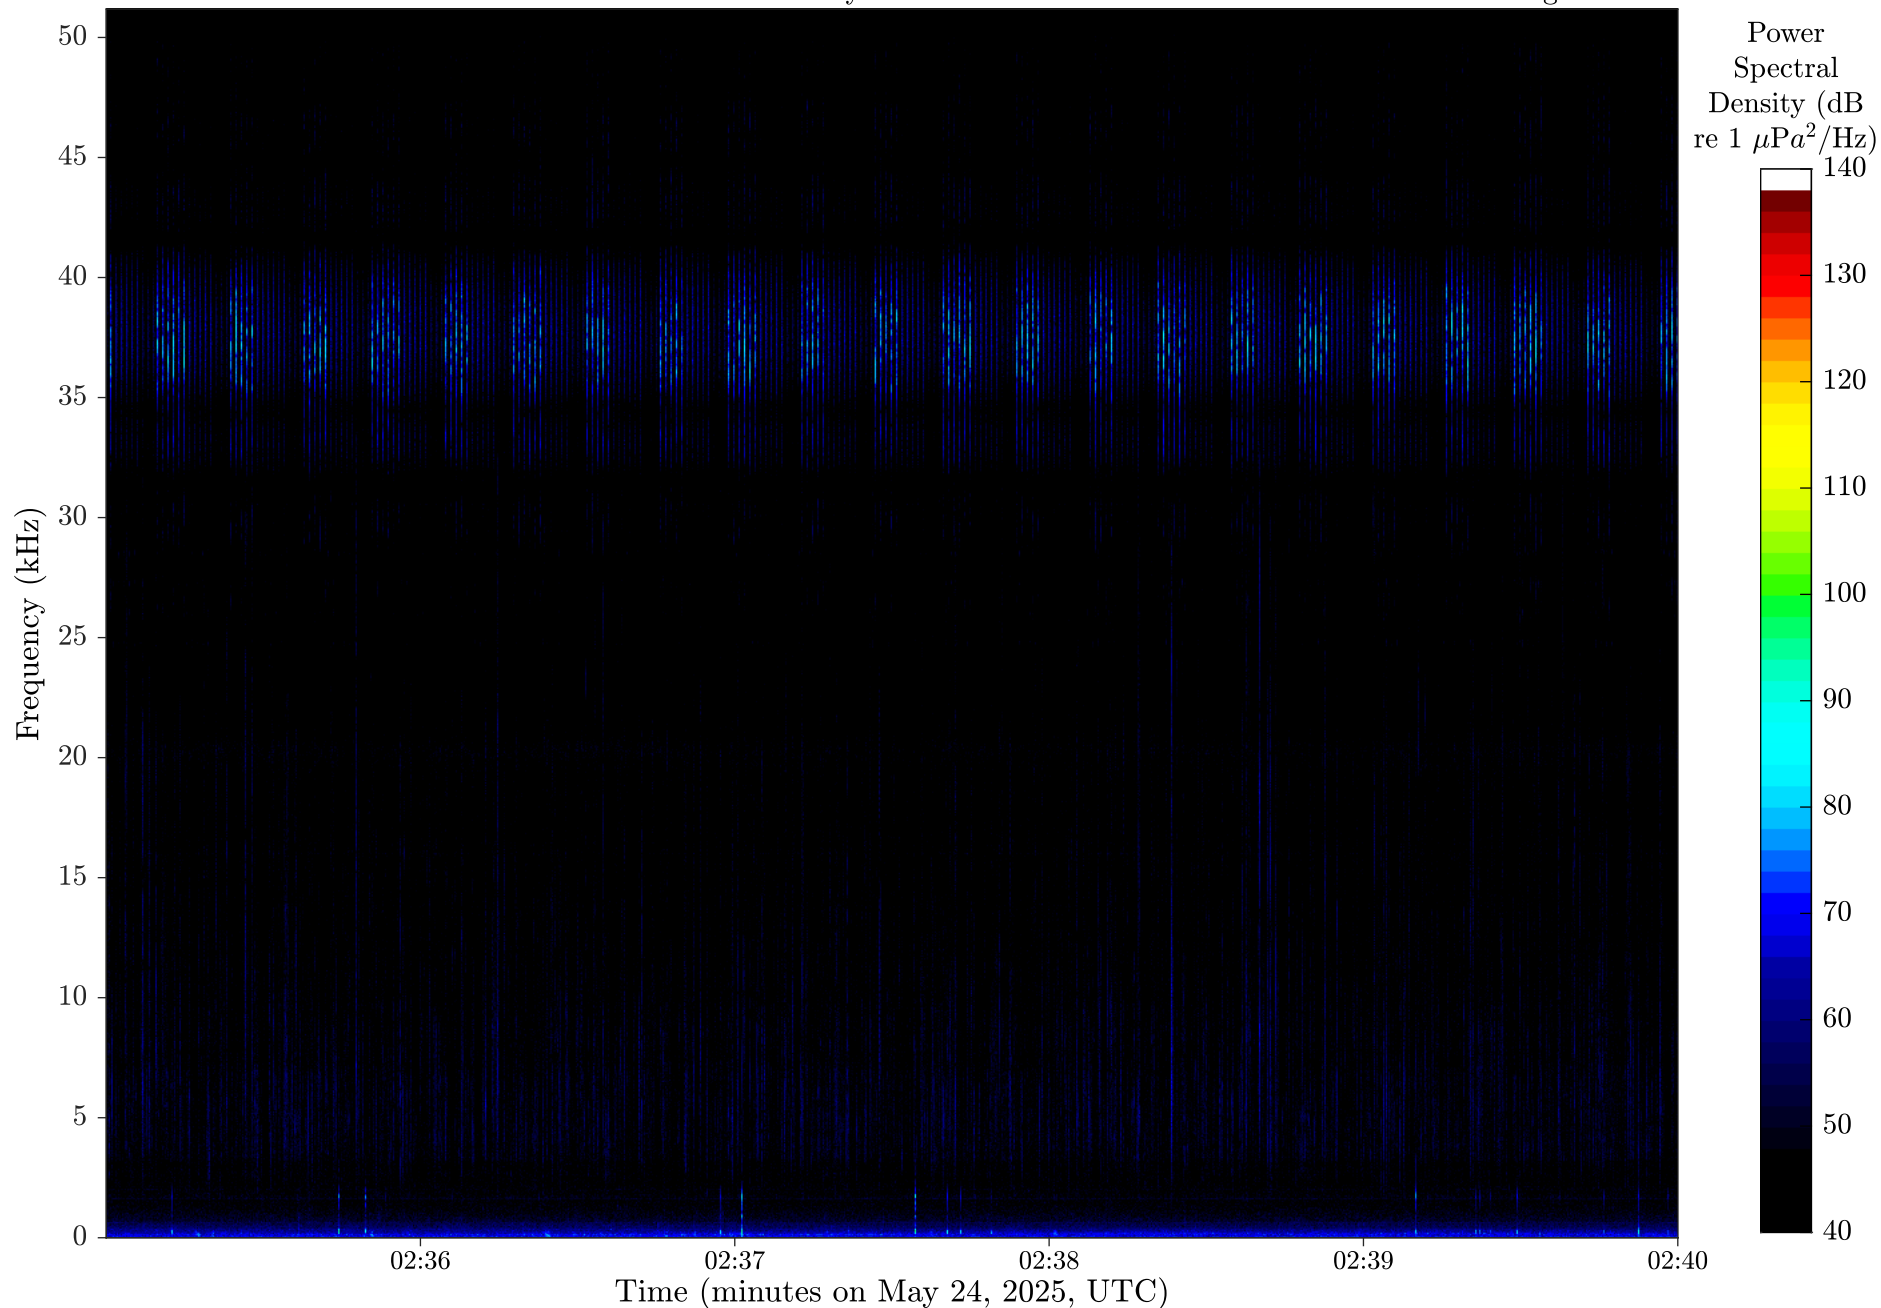

Comments: 36.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:16:00 UTC

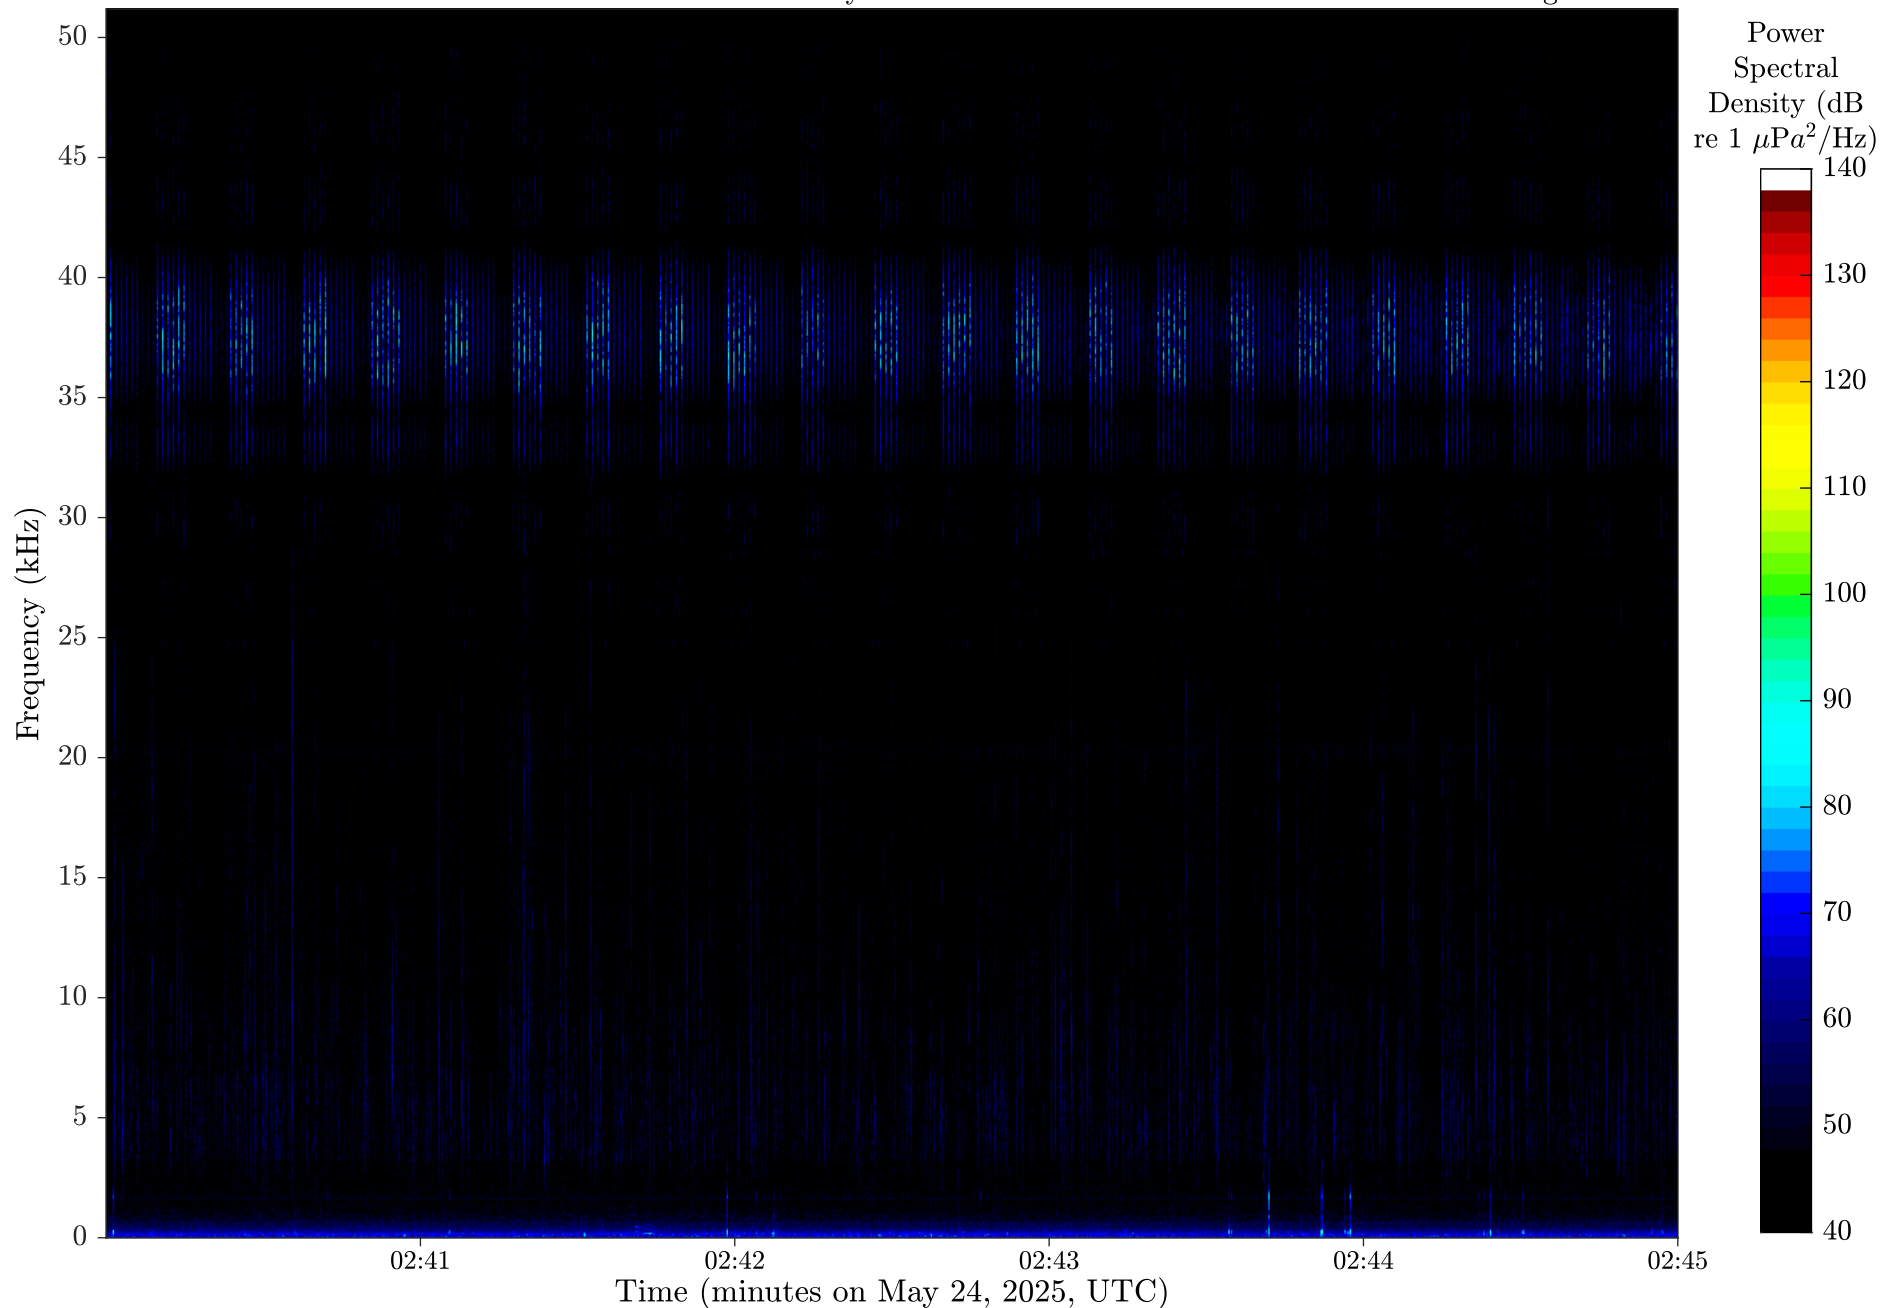

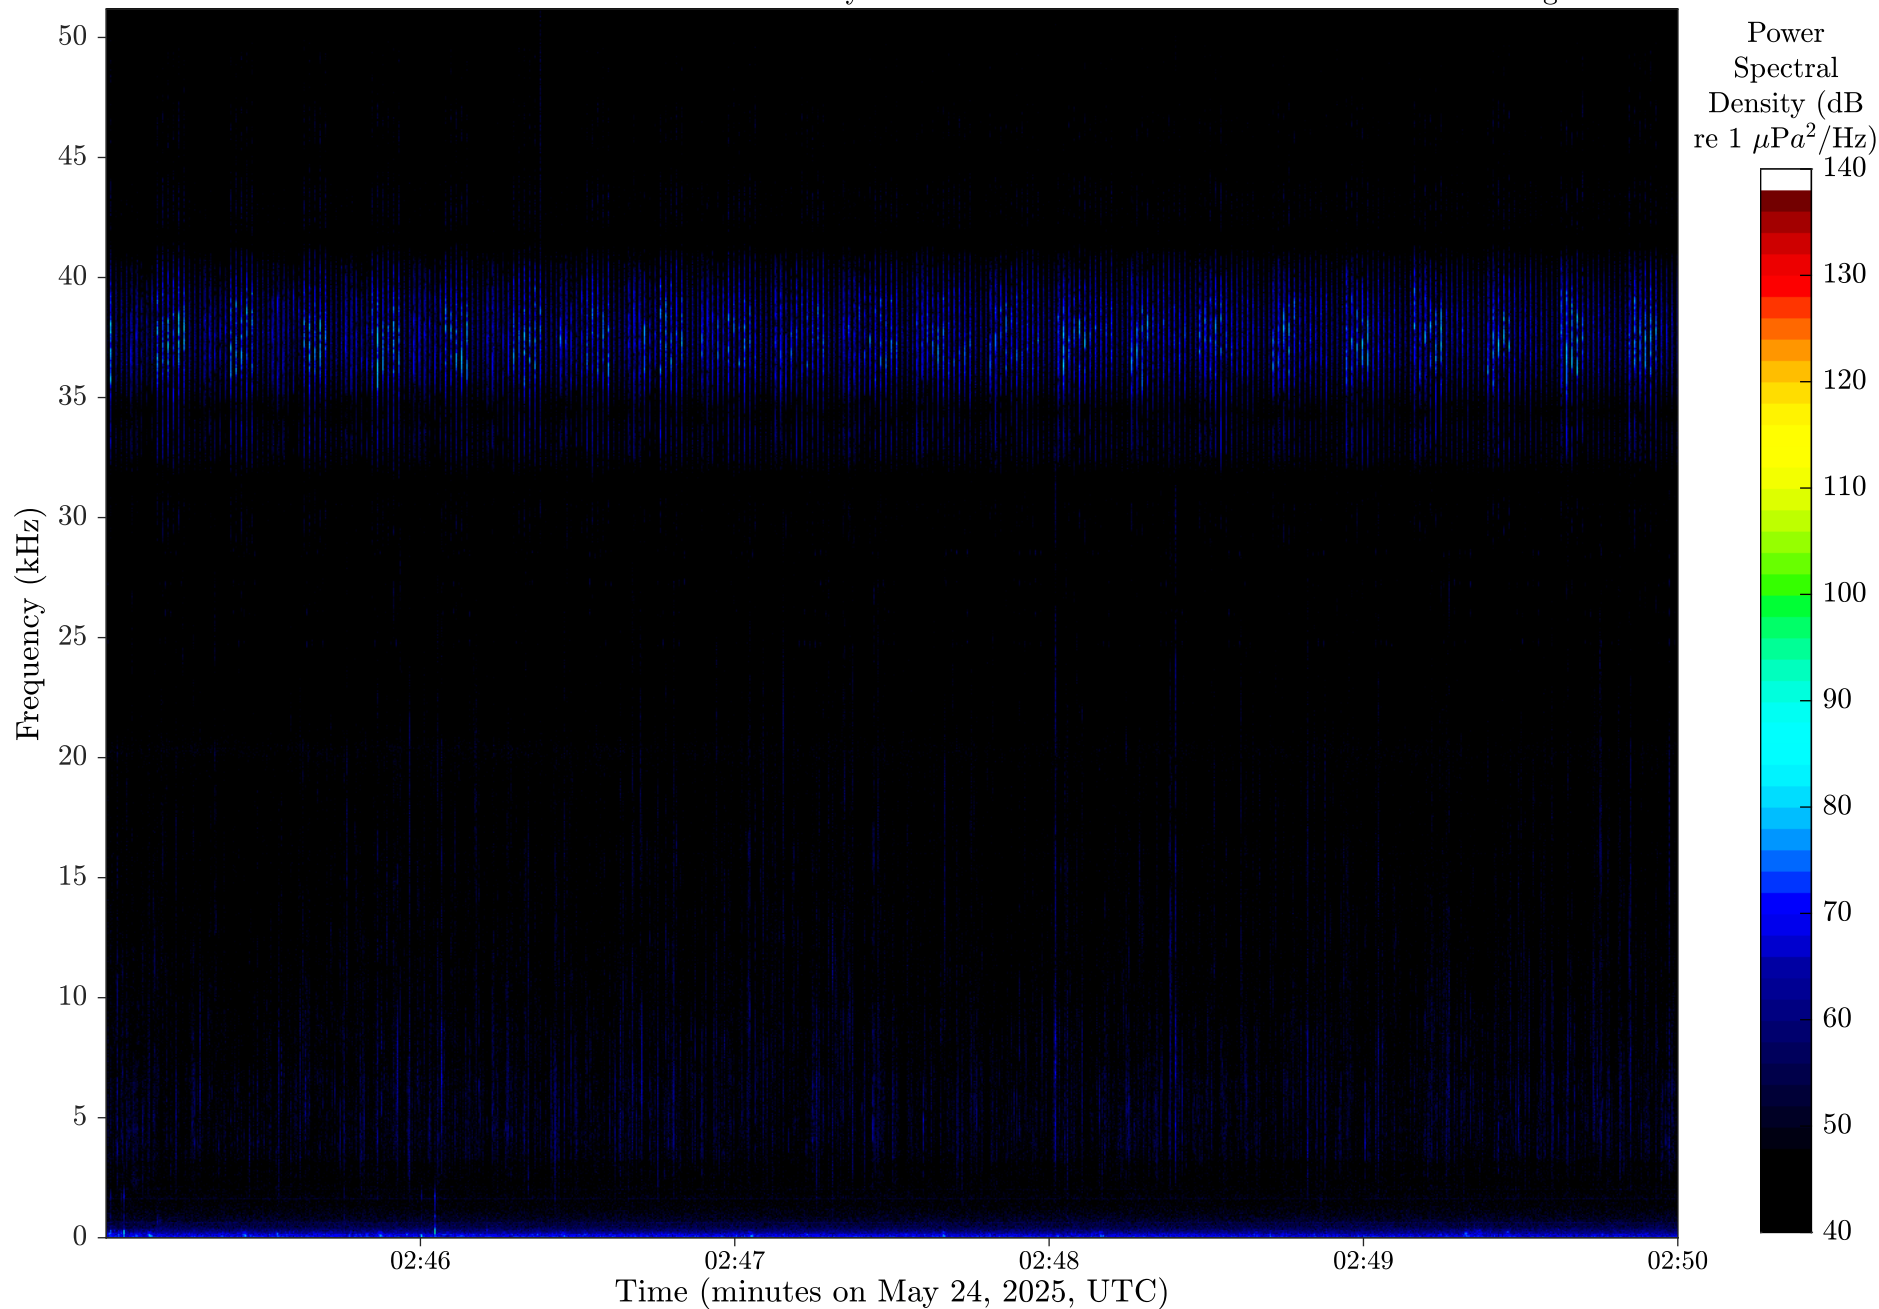


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:16:15 UTC

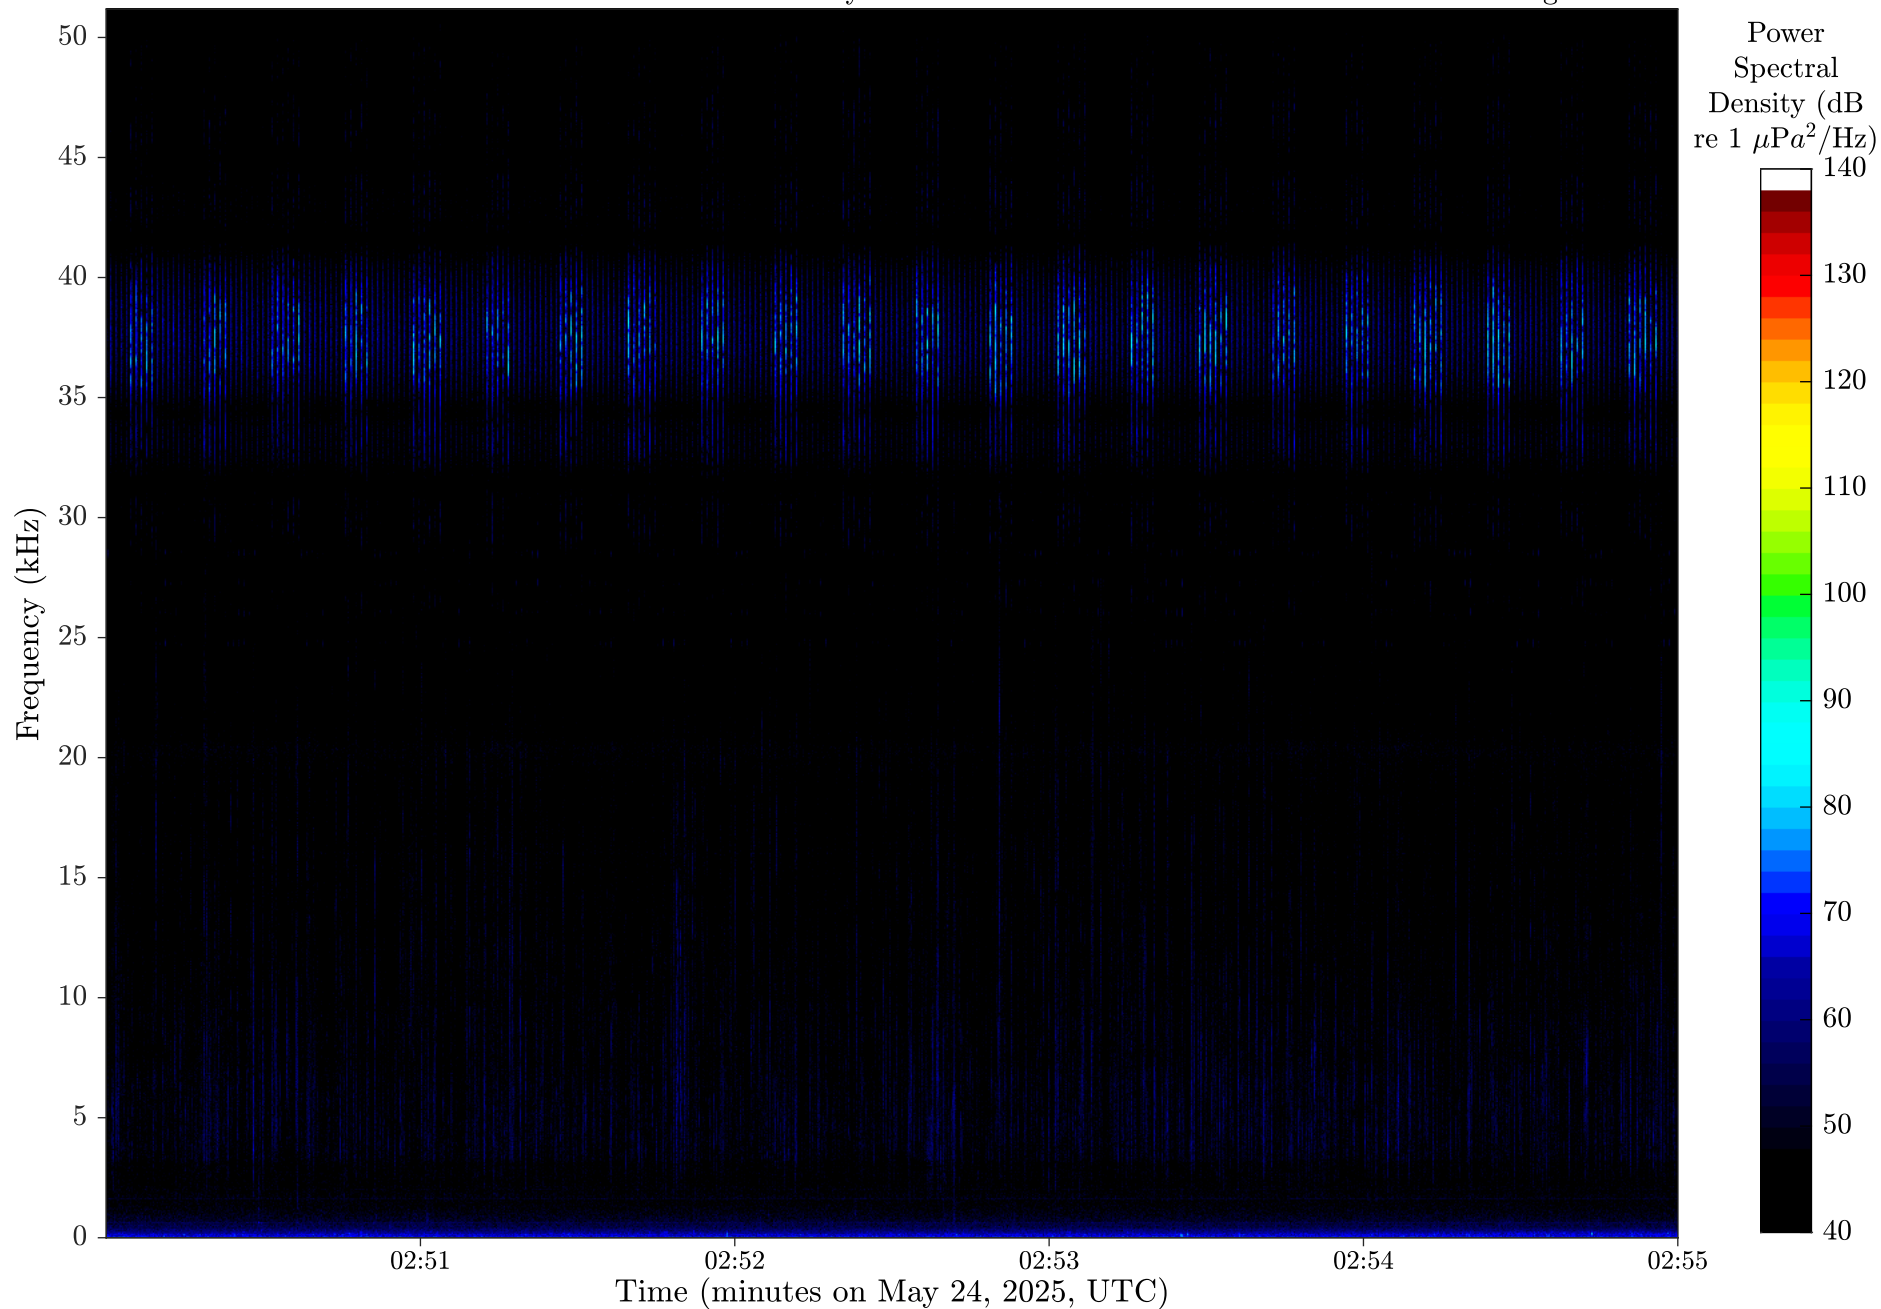


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:16:22 UTC

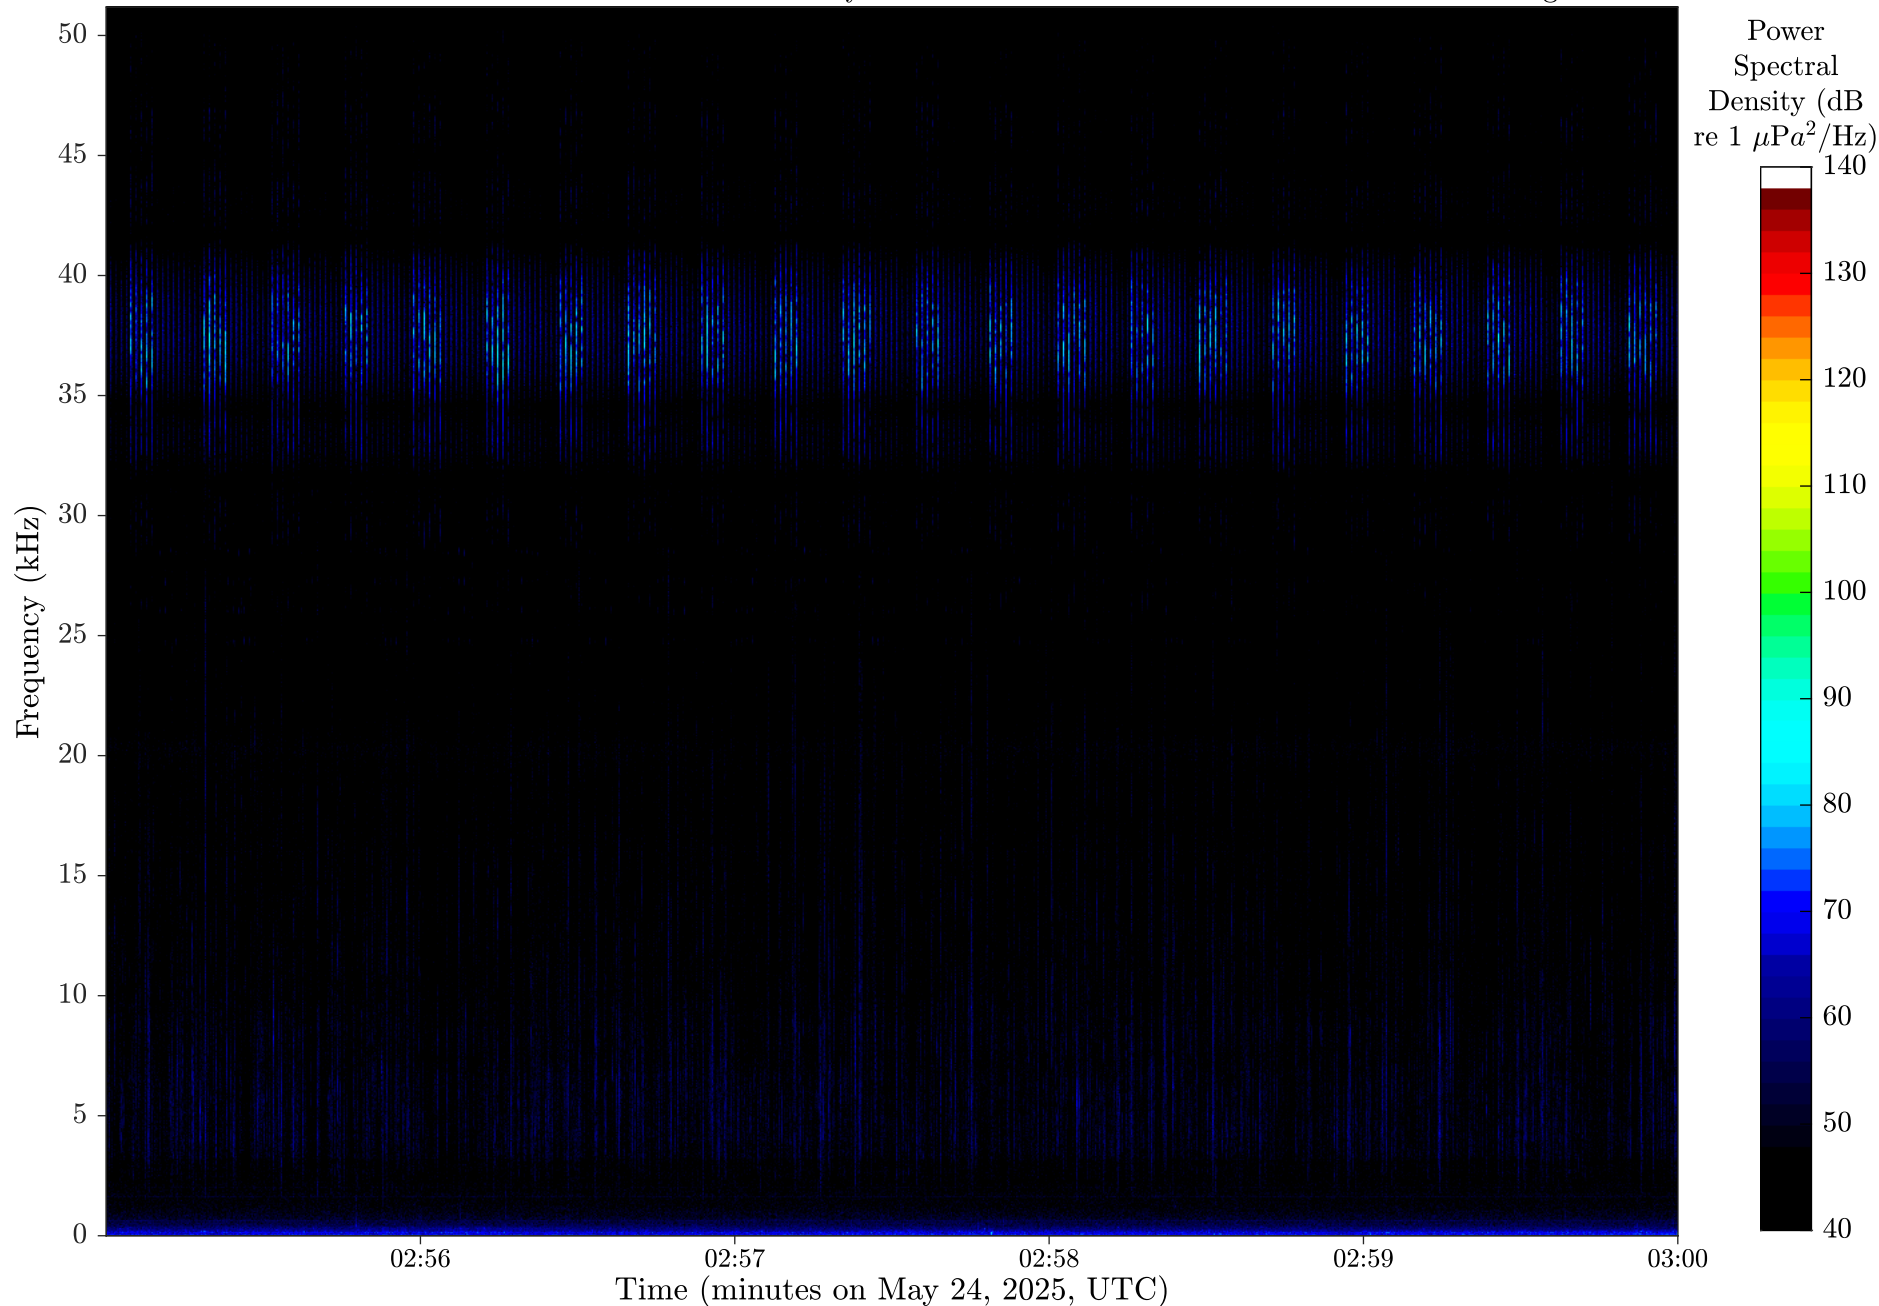


Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:16:29 UTC

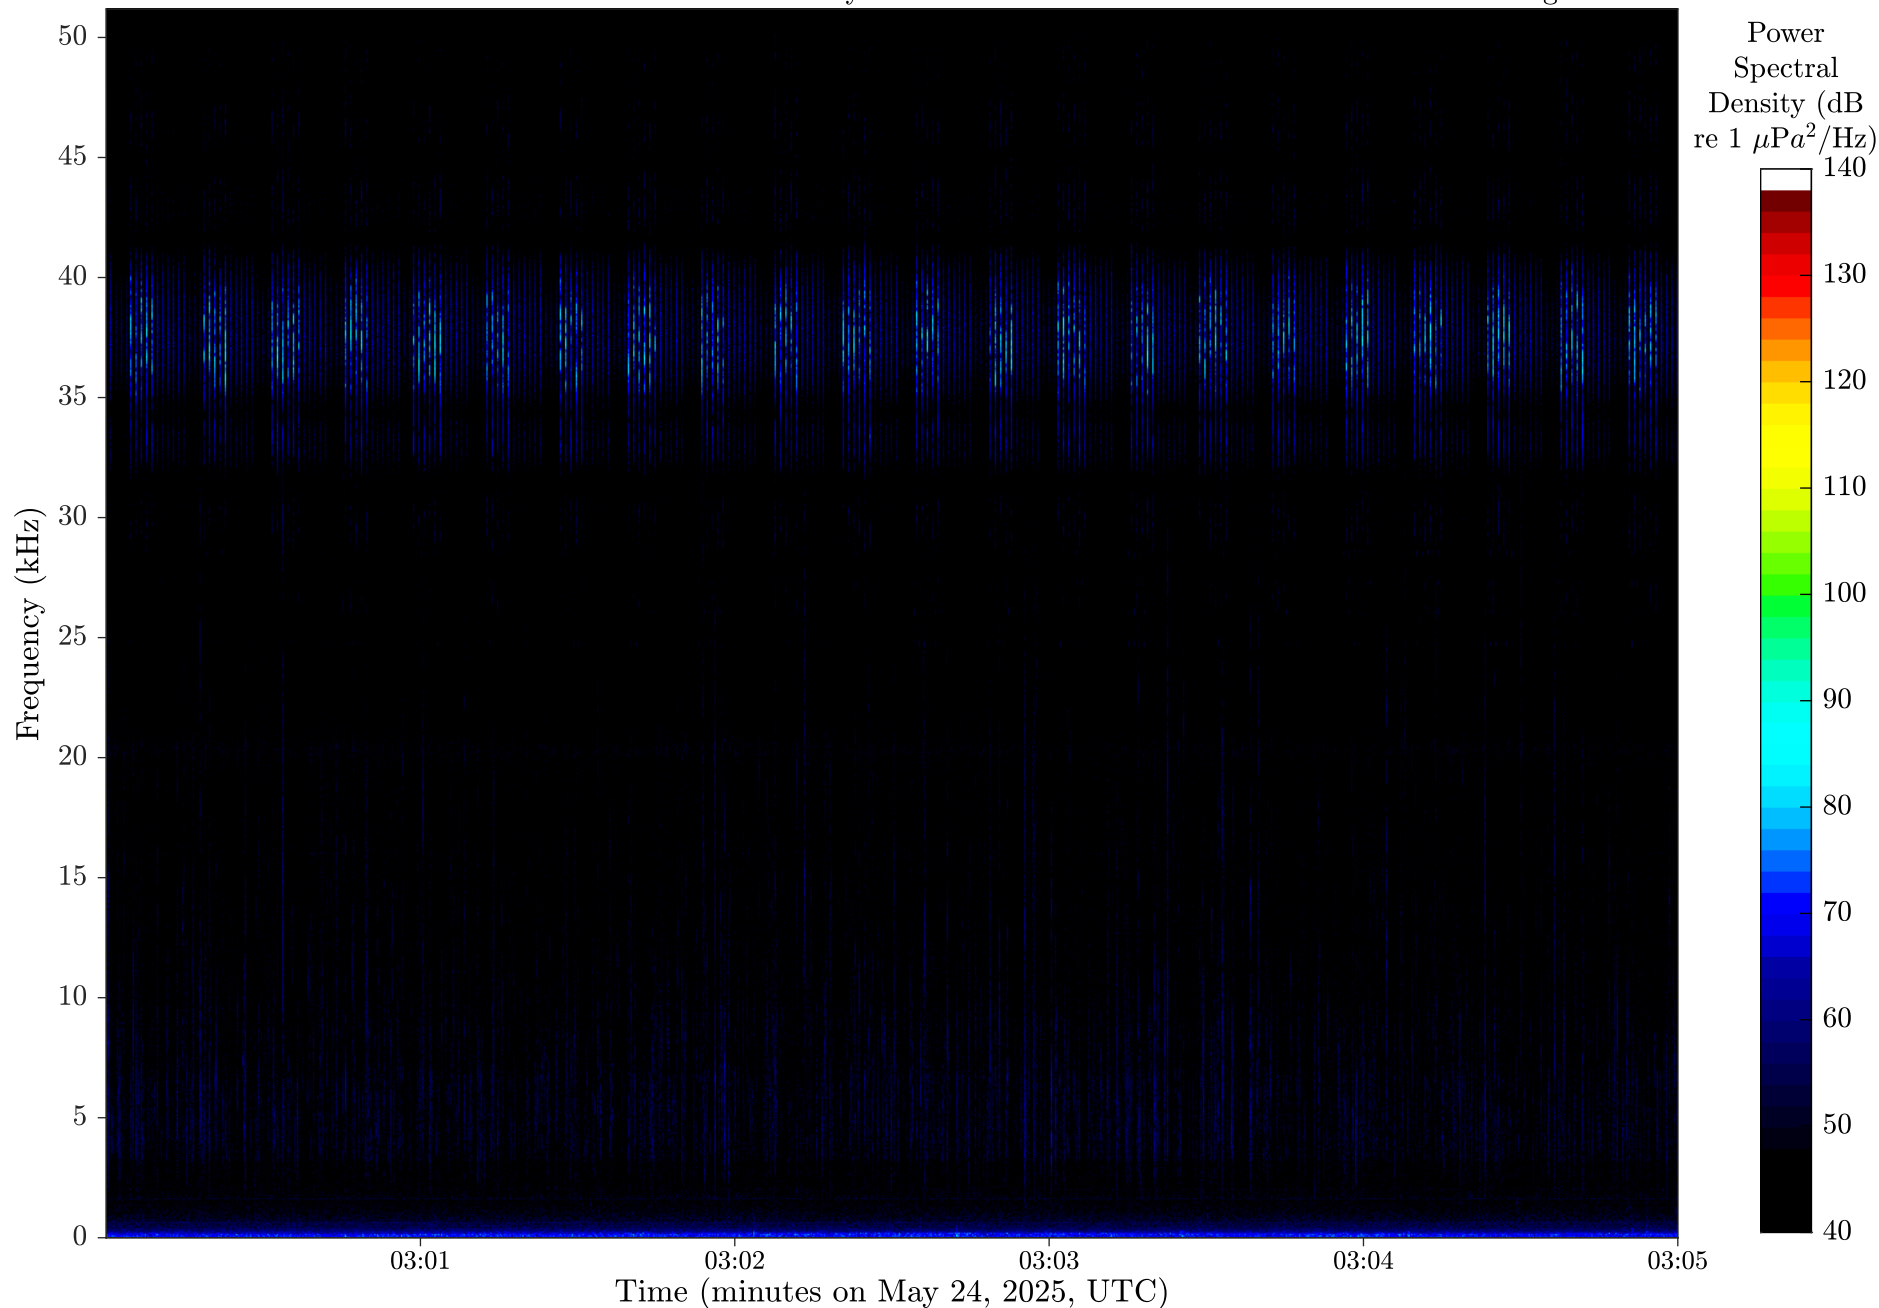


Comments: 35.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:16:36 UTC

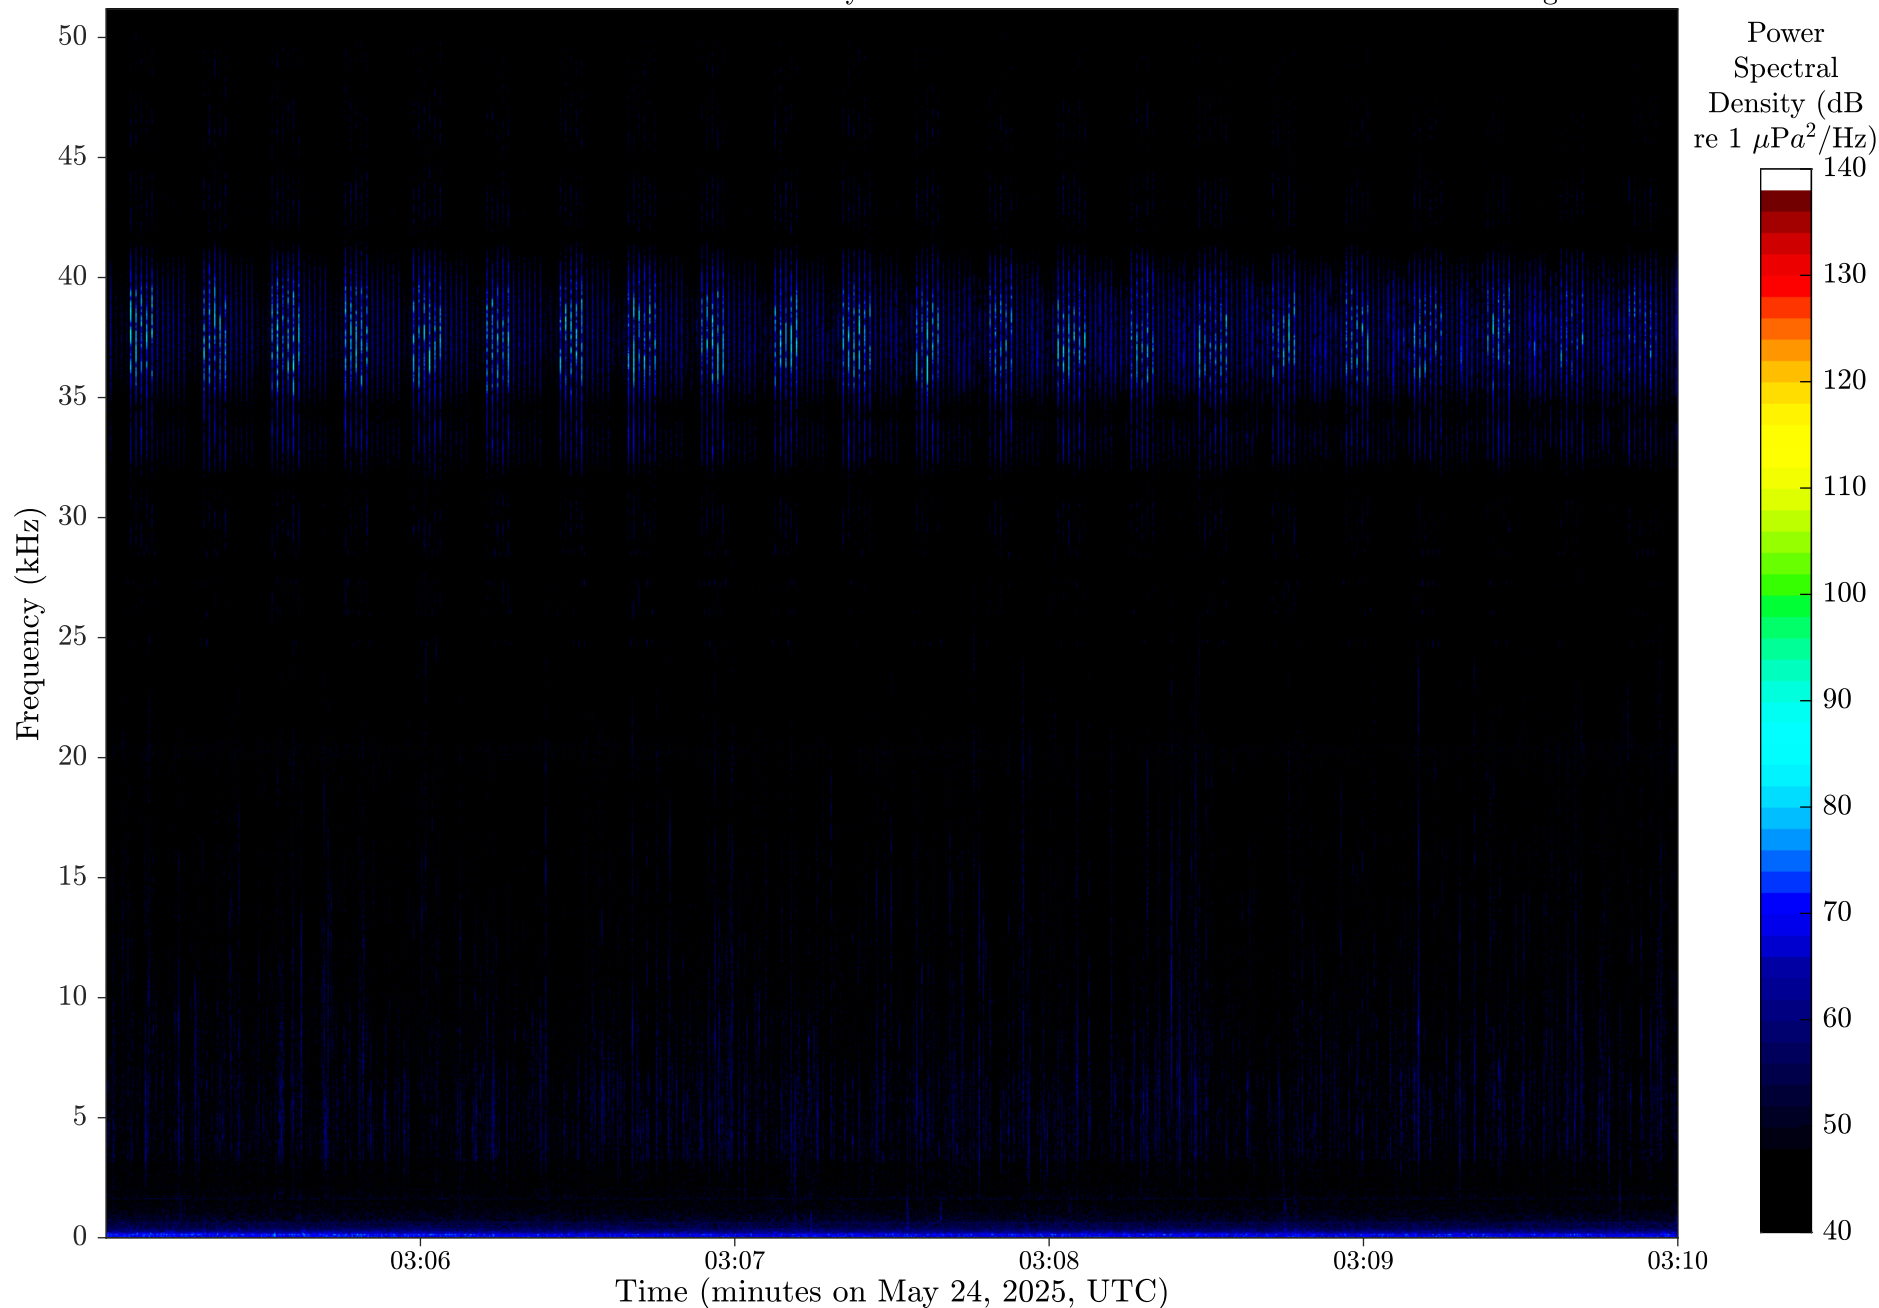


Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:16:44 UTC

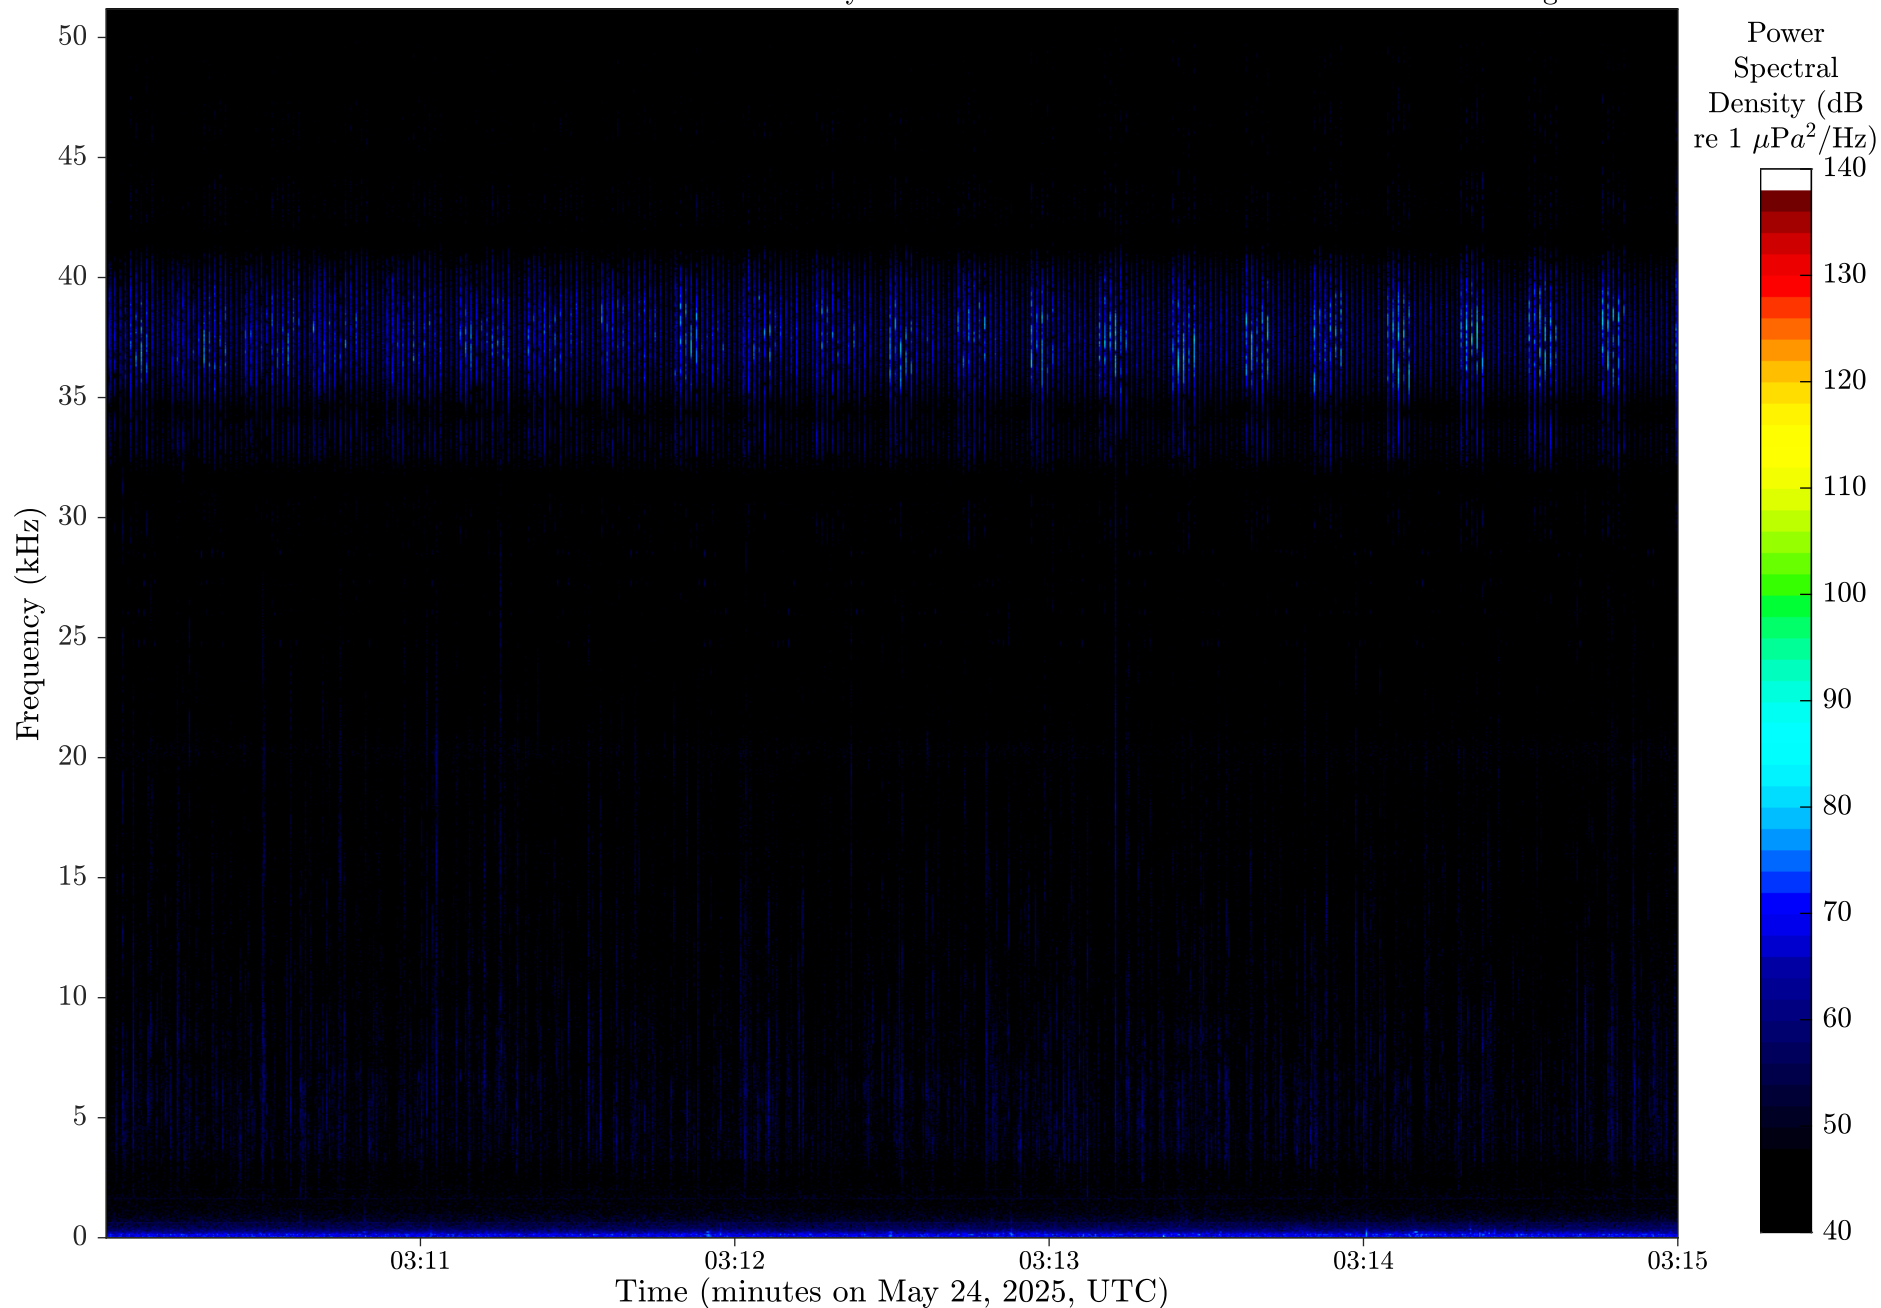


Comments: 33.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:16:51 UTC

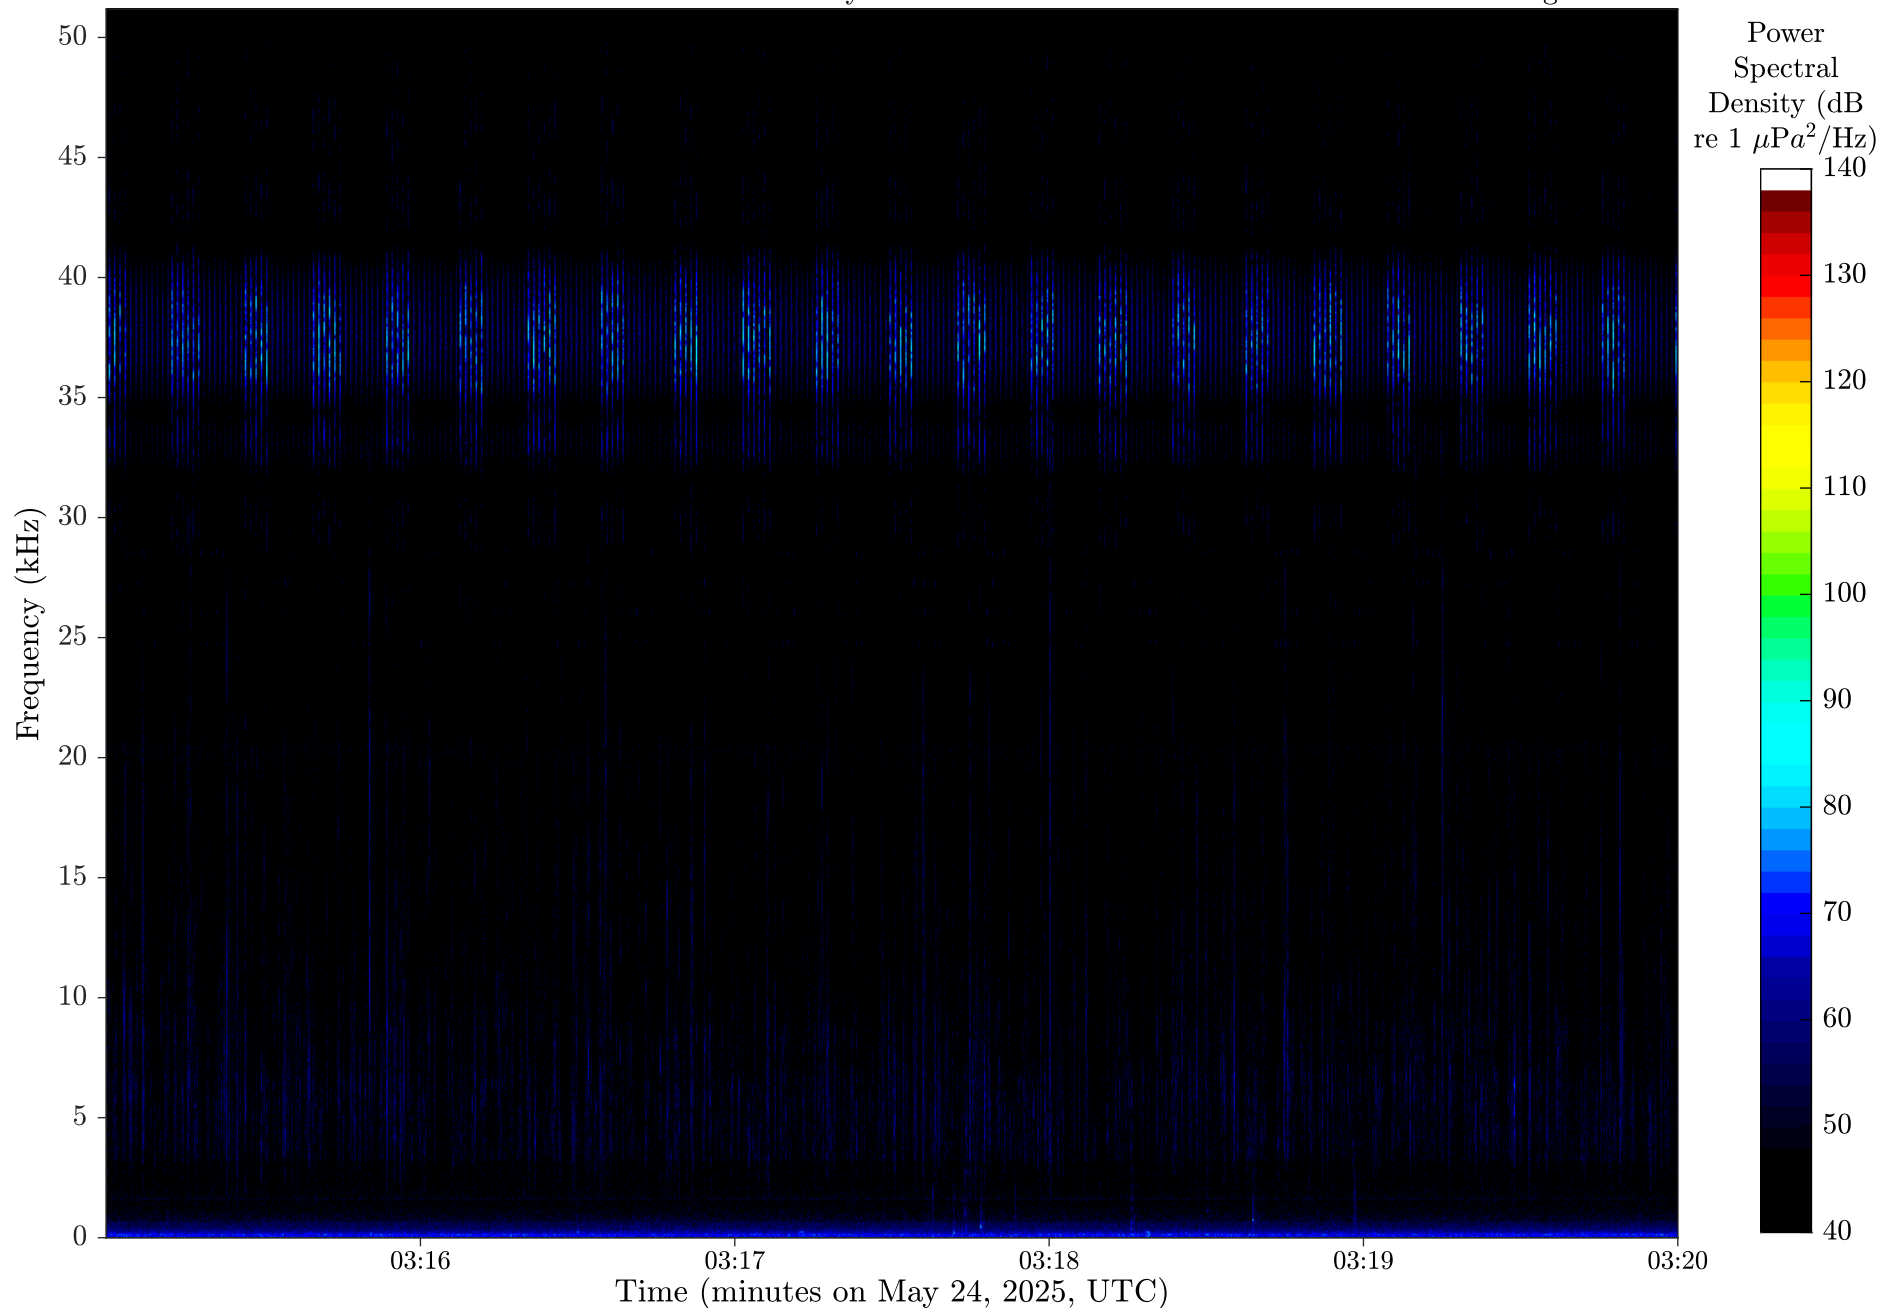


Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:16:58 UTC

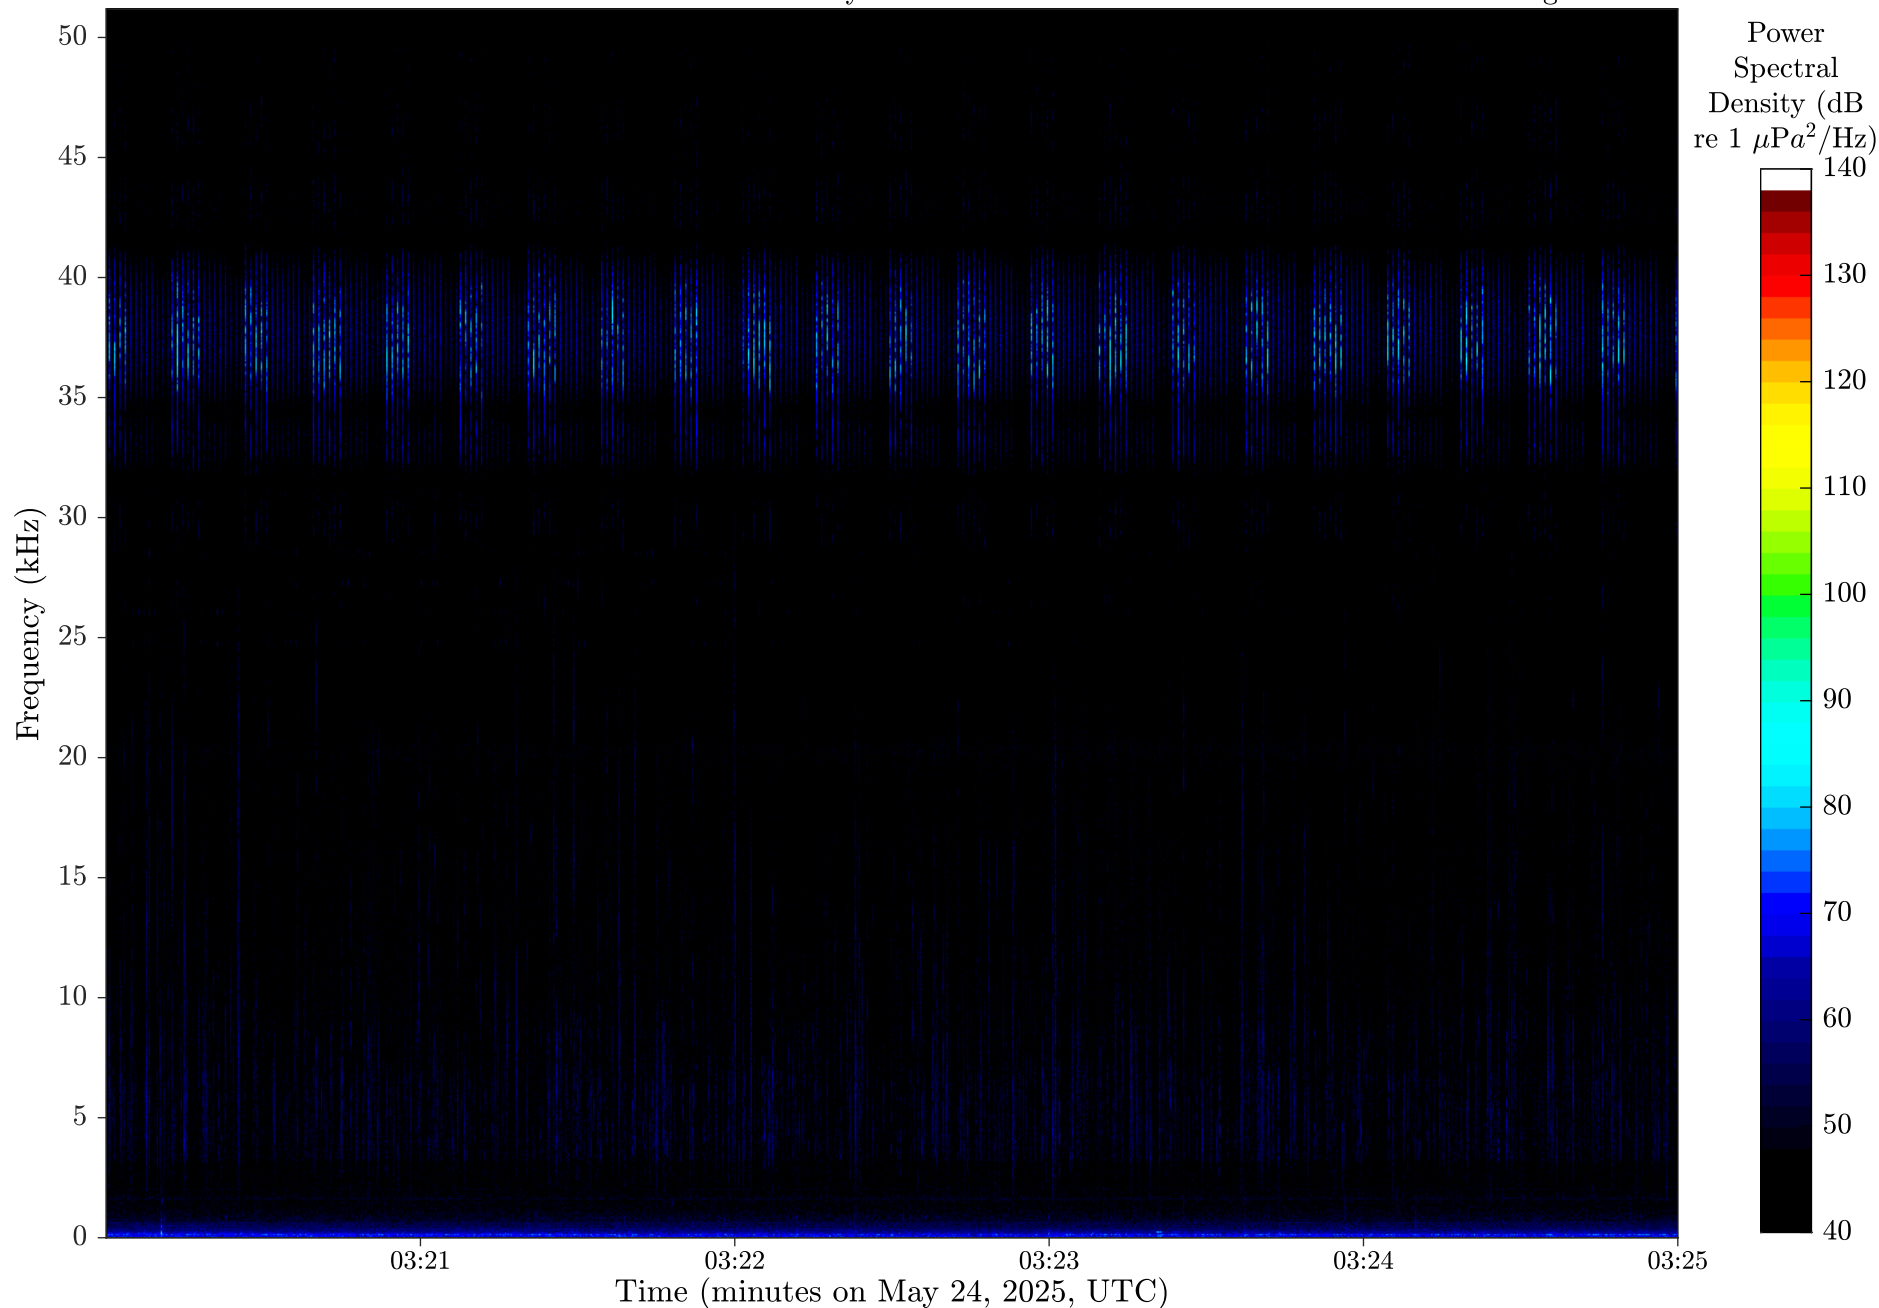


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:17:06 UTC

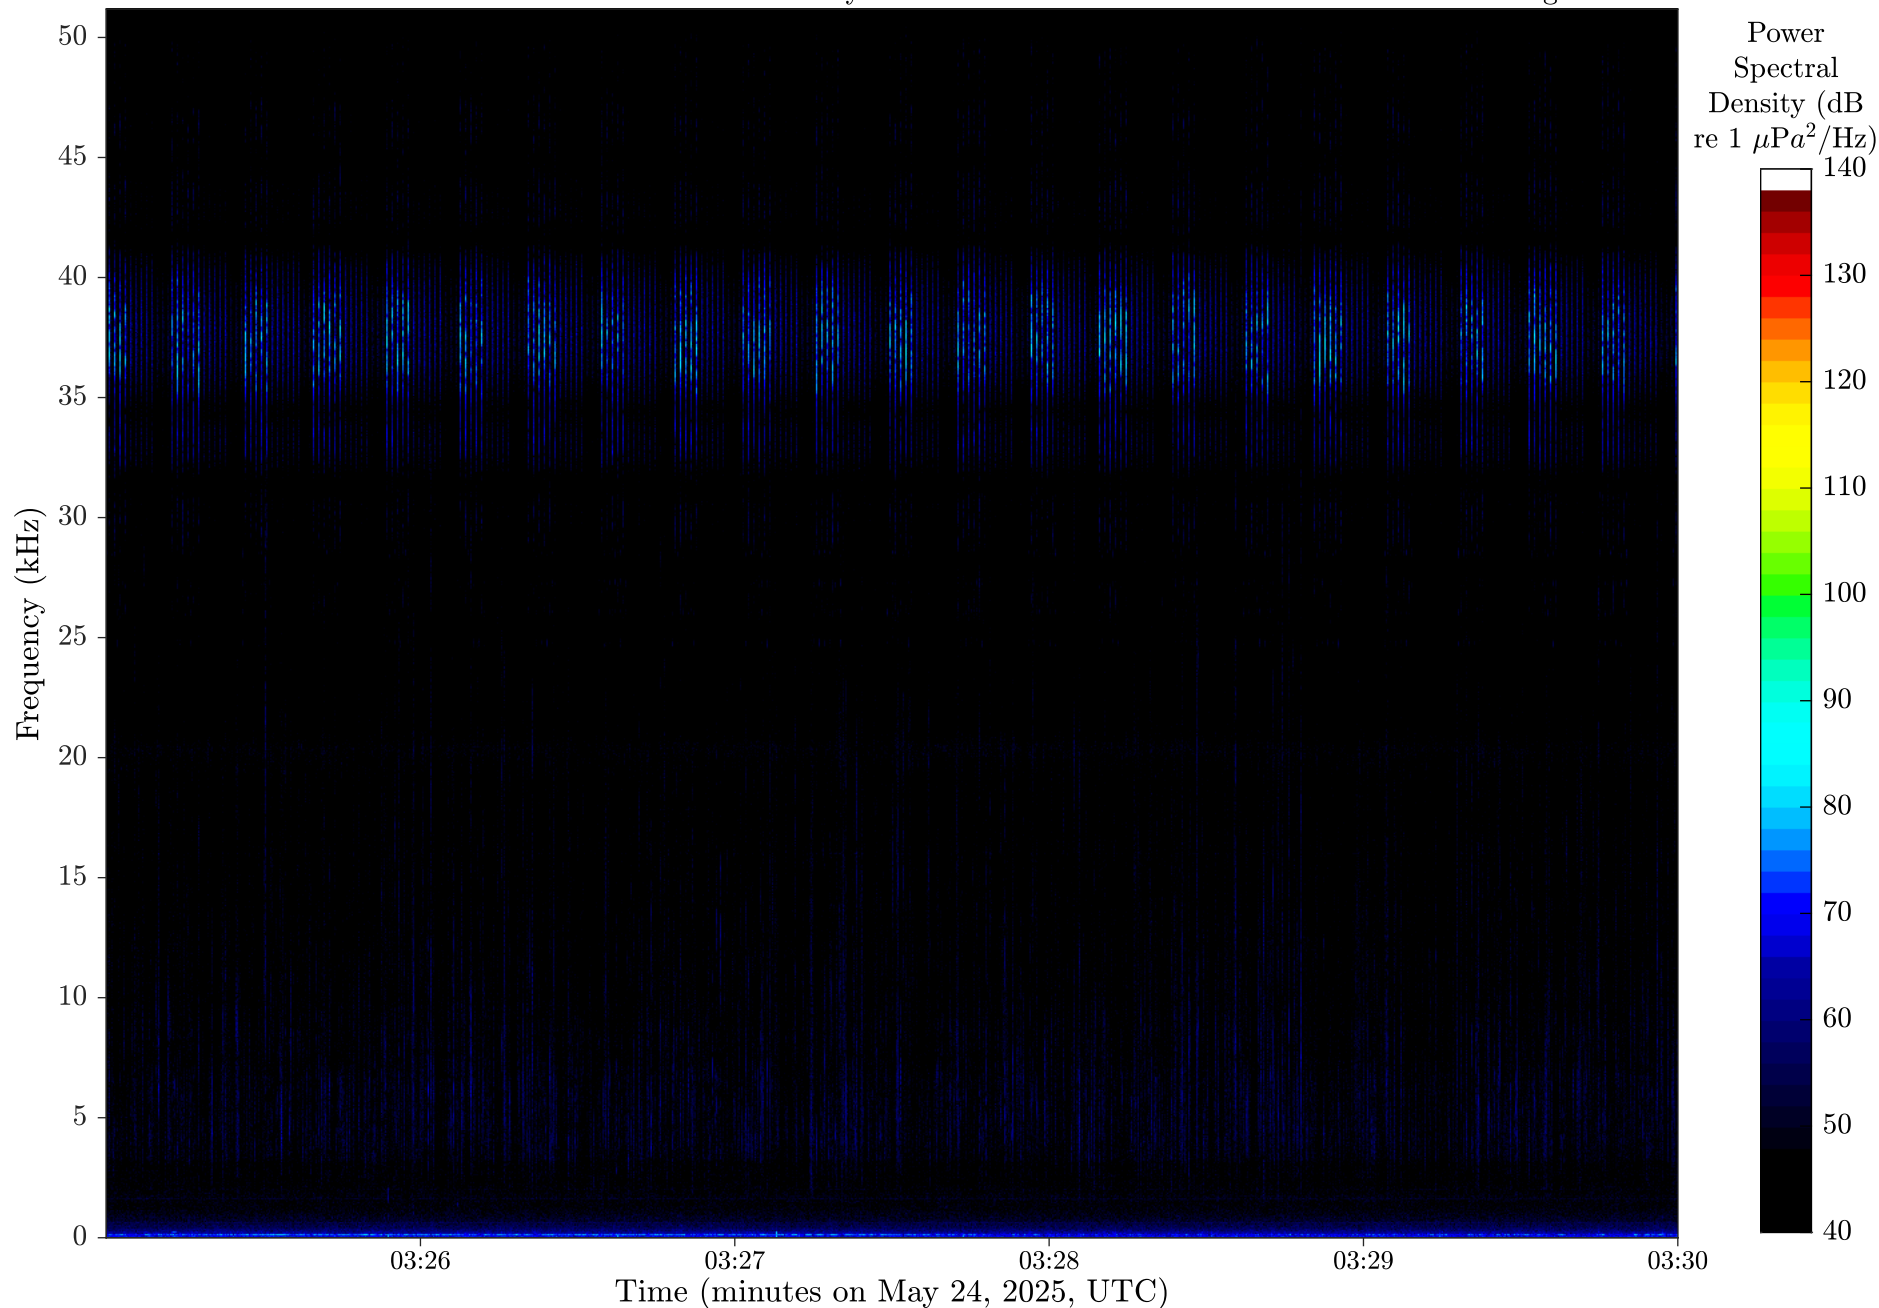


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:17:13 UTC

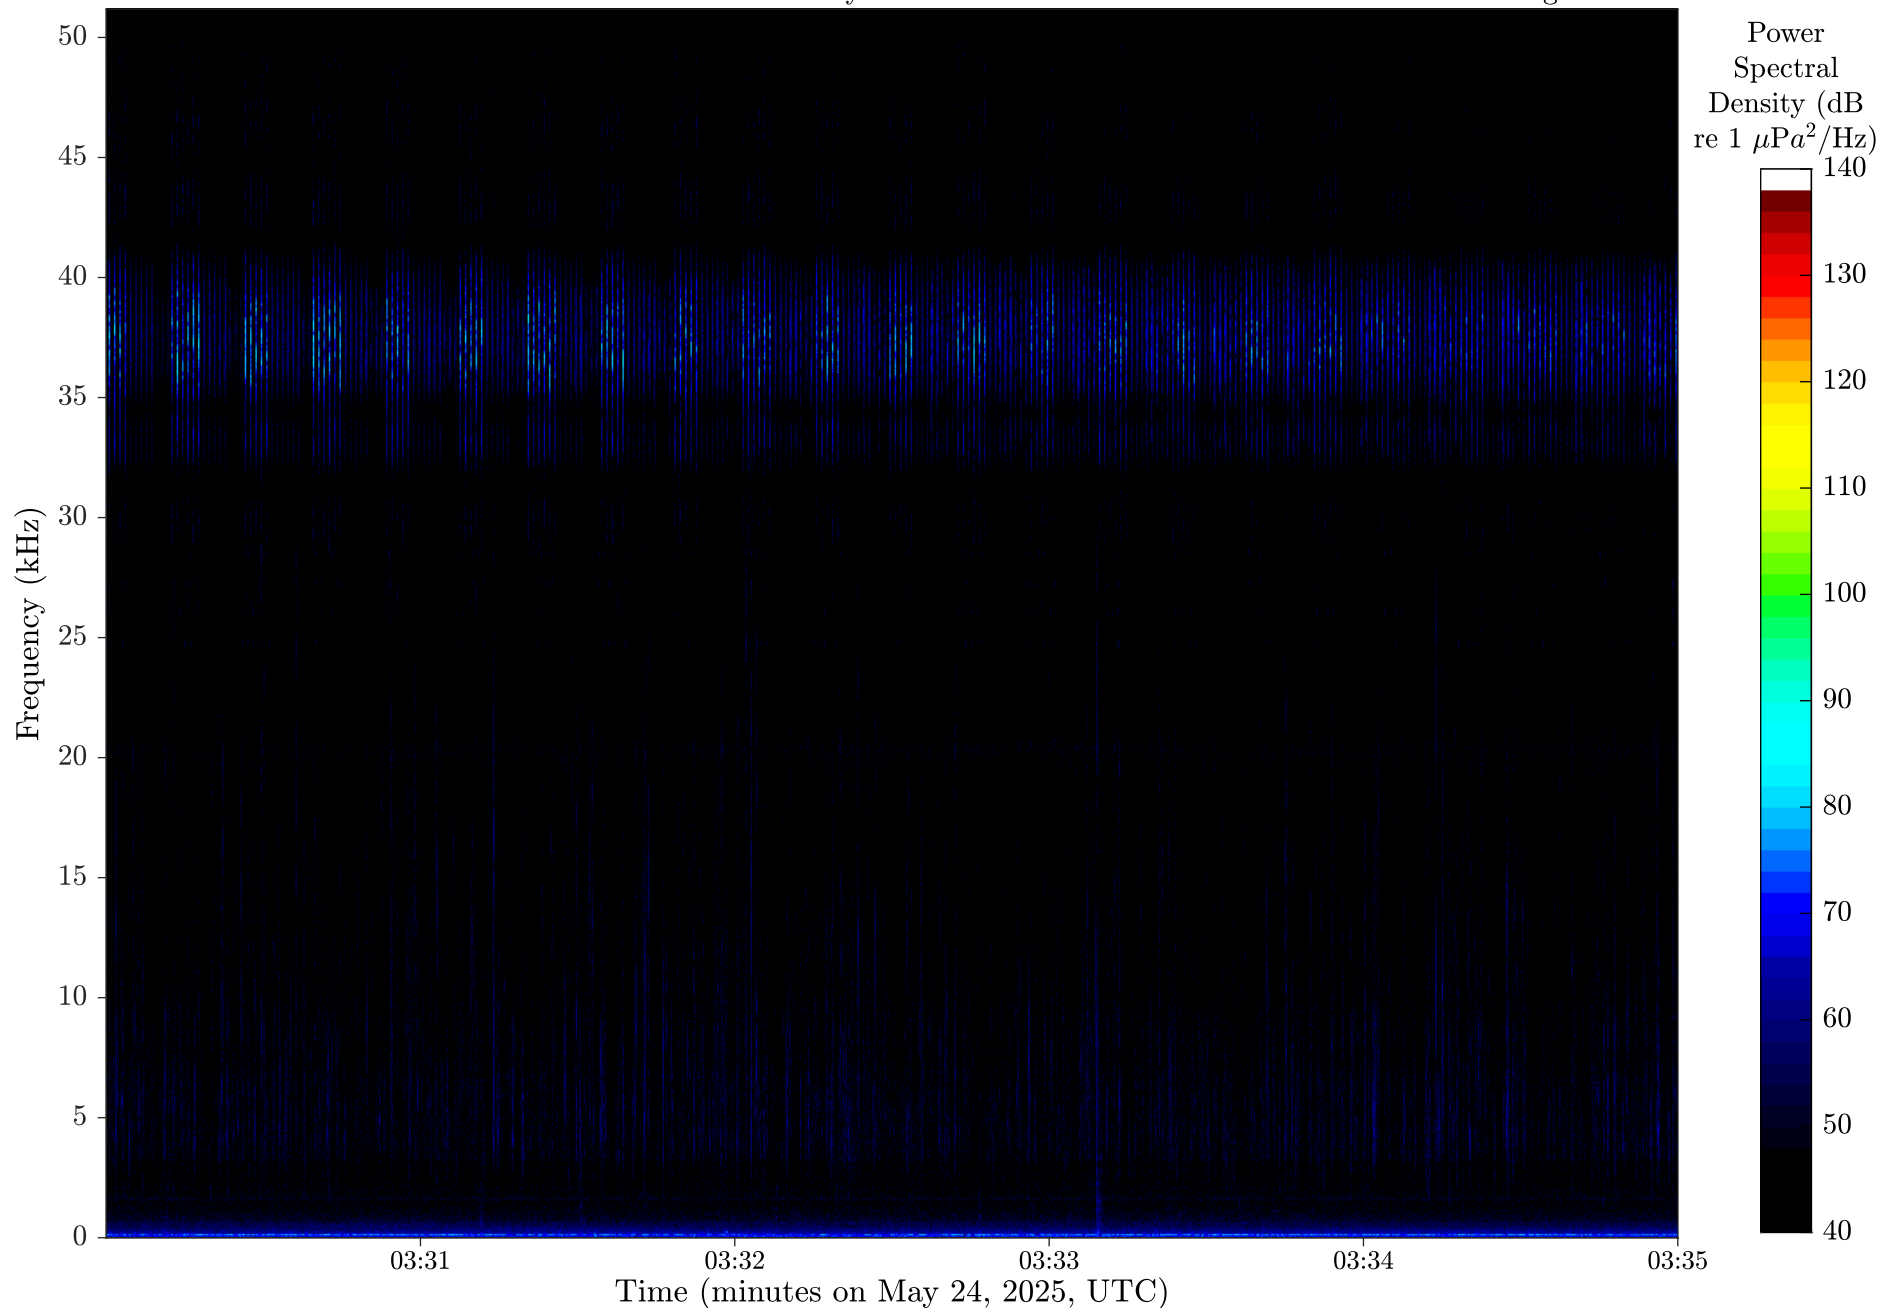


Comments: 34.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:17:20 UTC

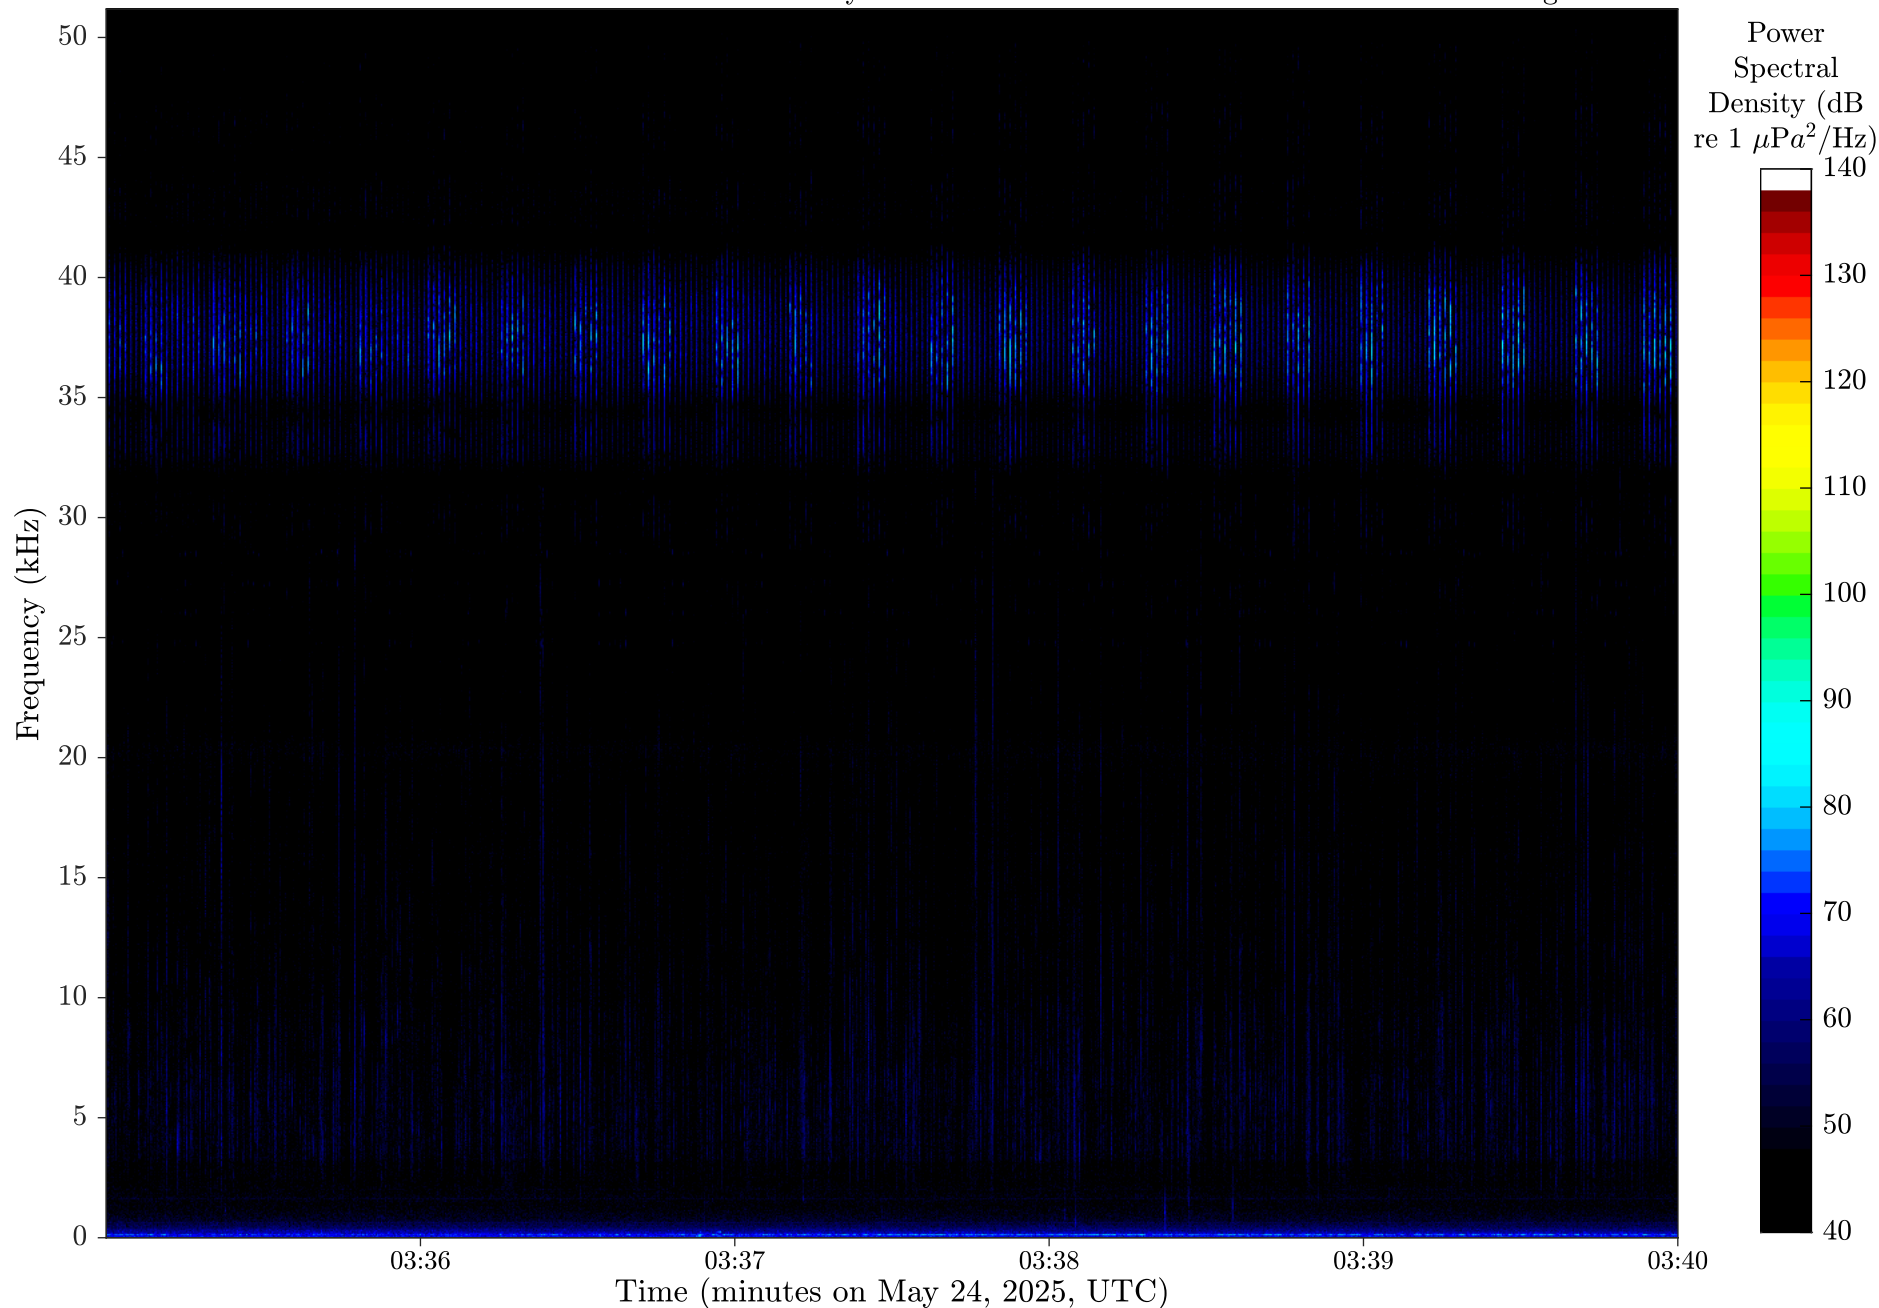


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:17:28 UTC

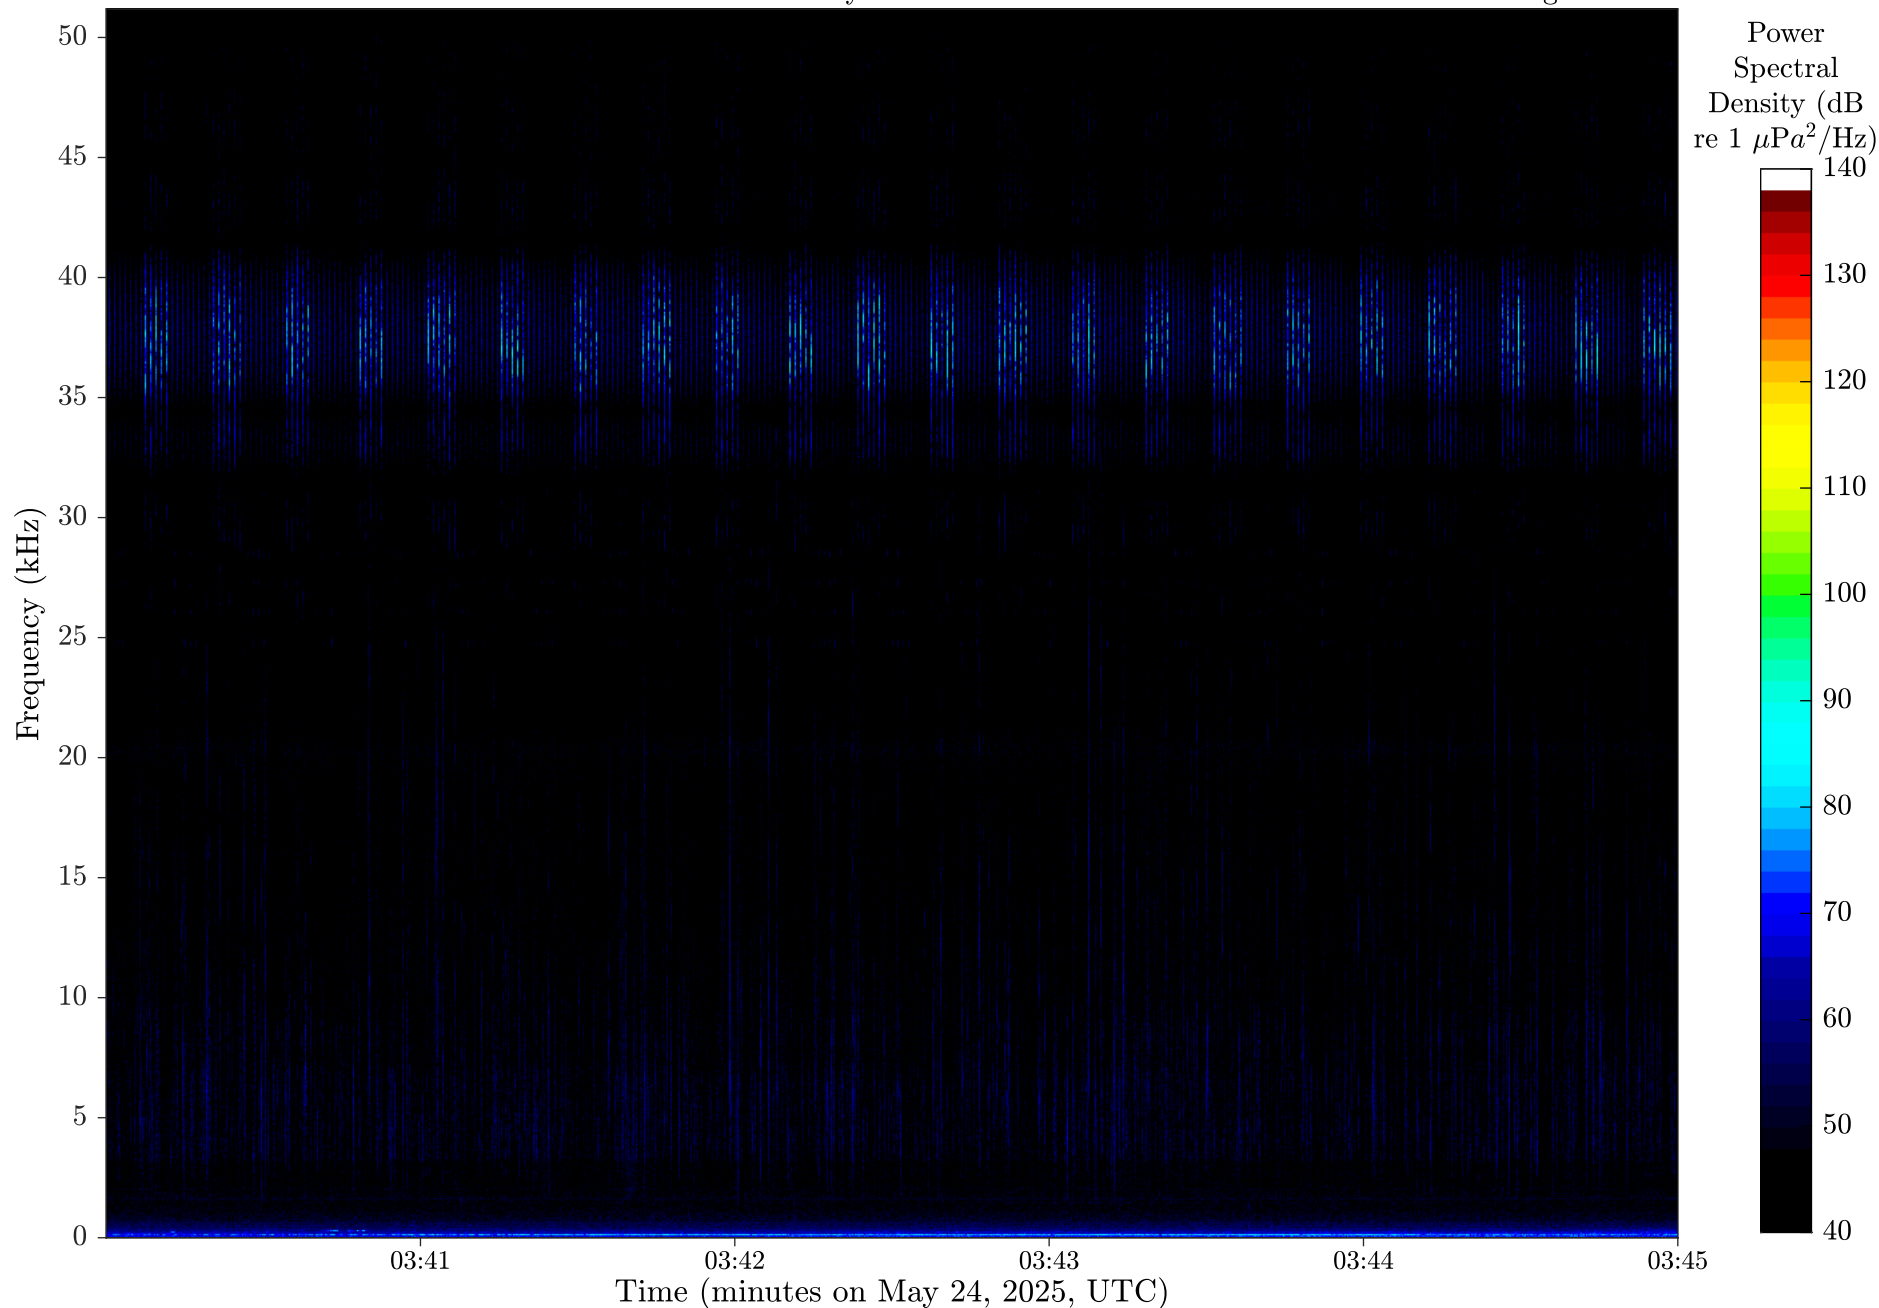


Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:17:35 UTC

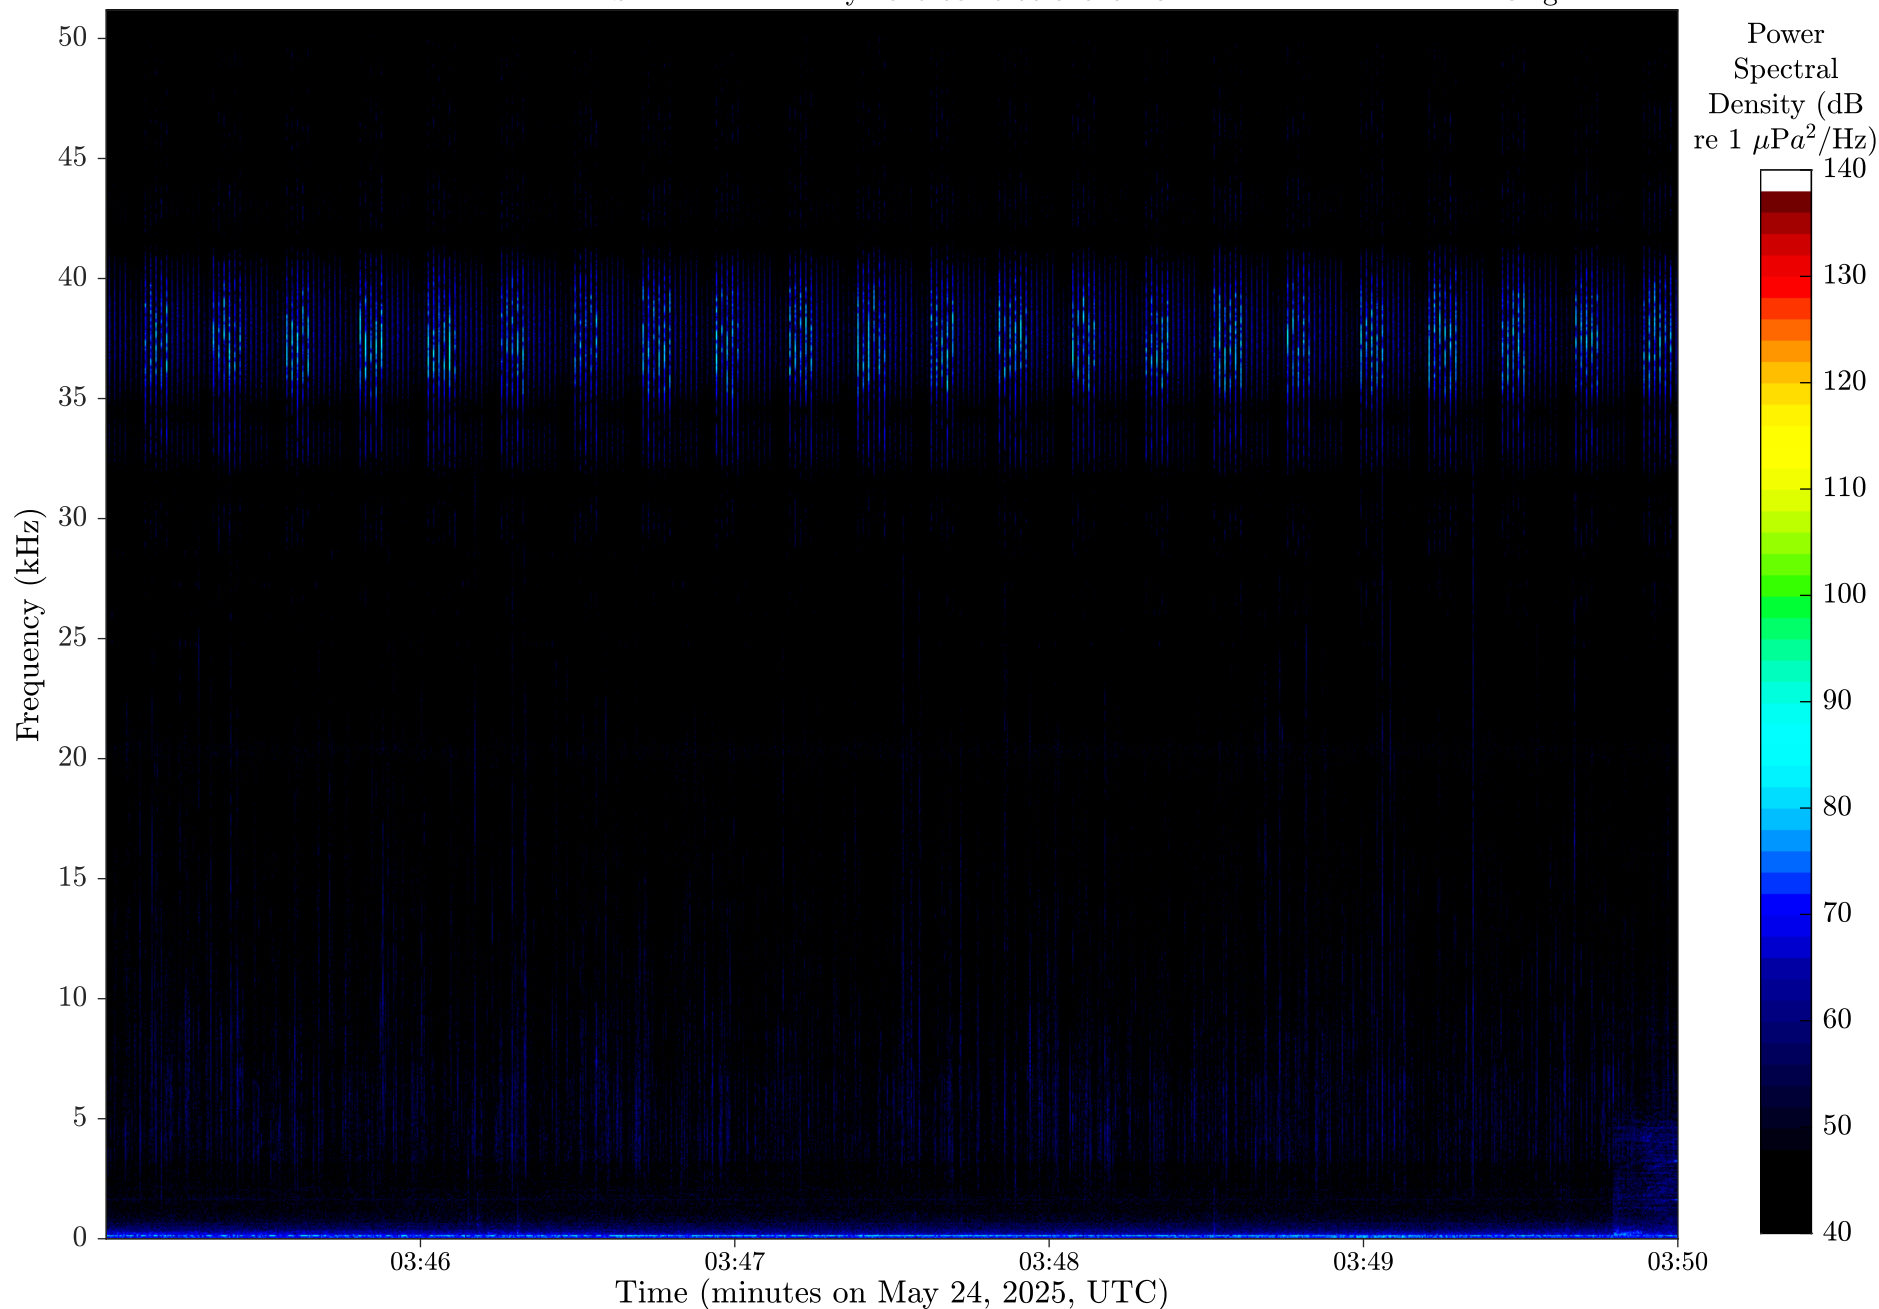


Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:17:42 UTC

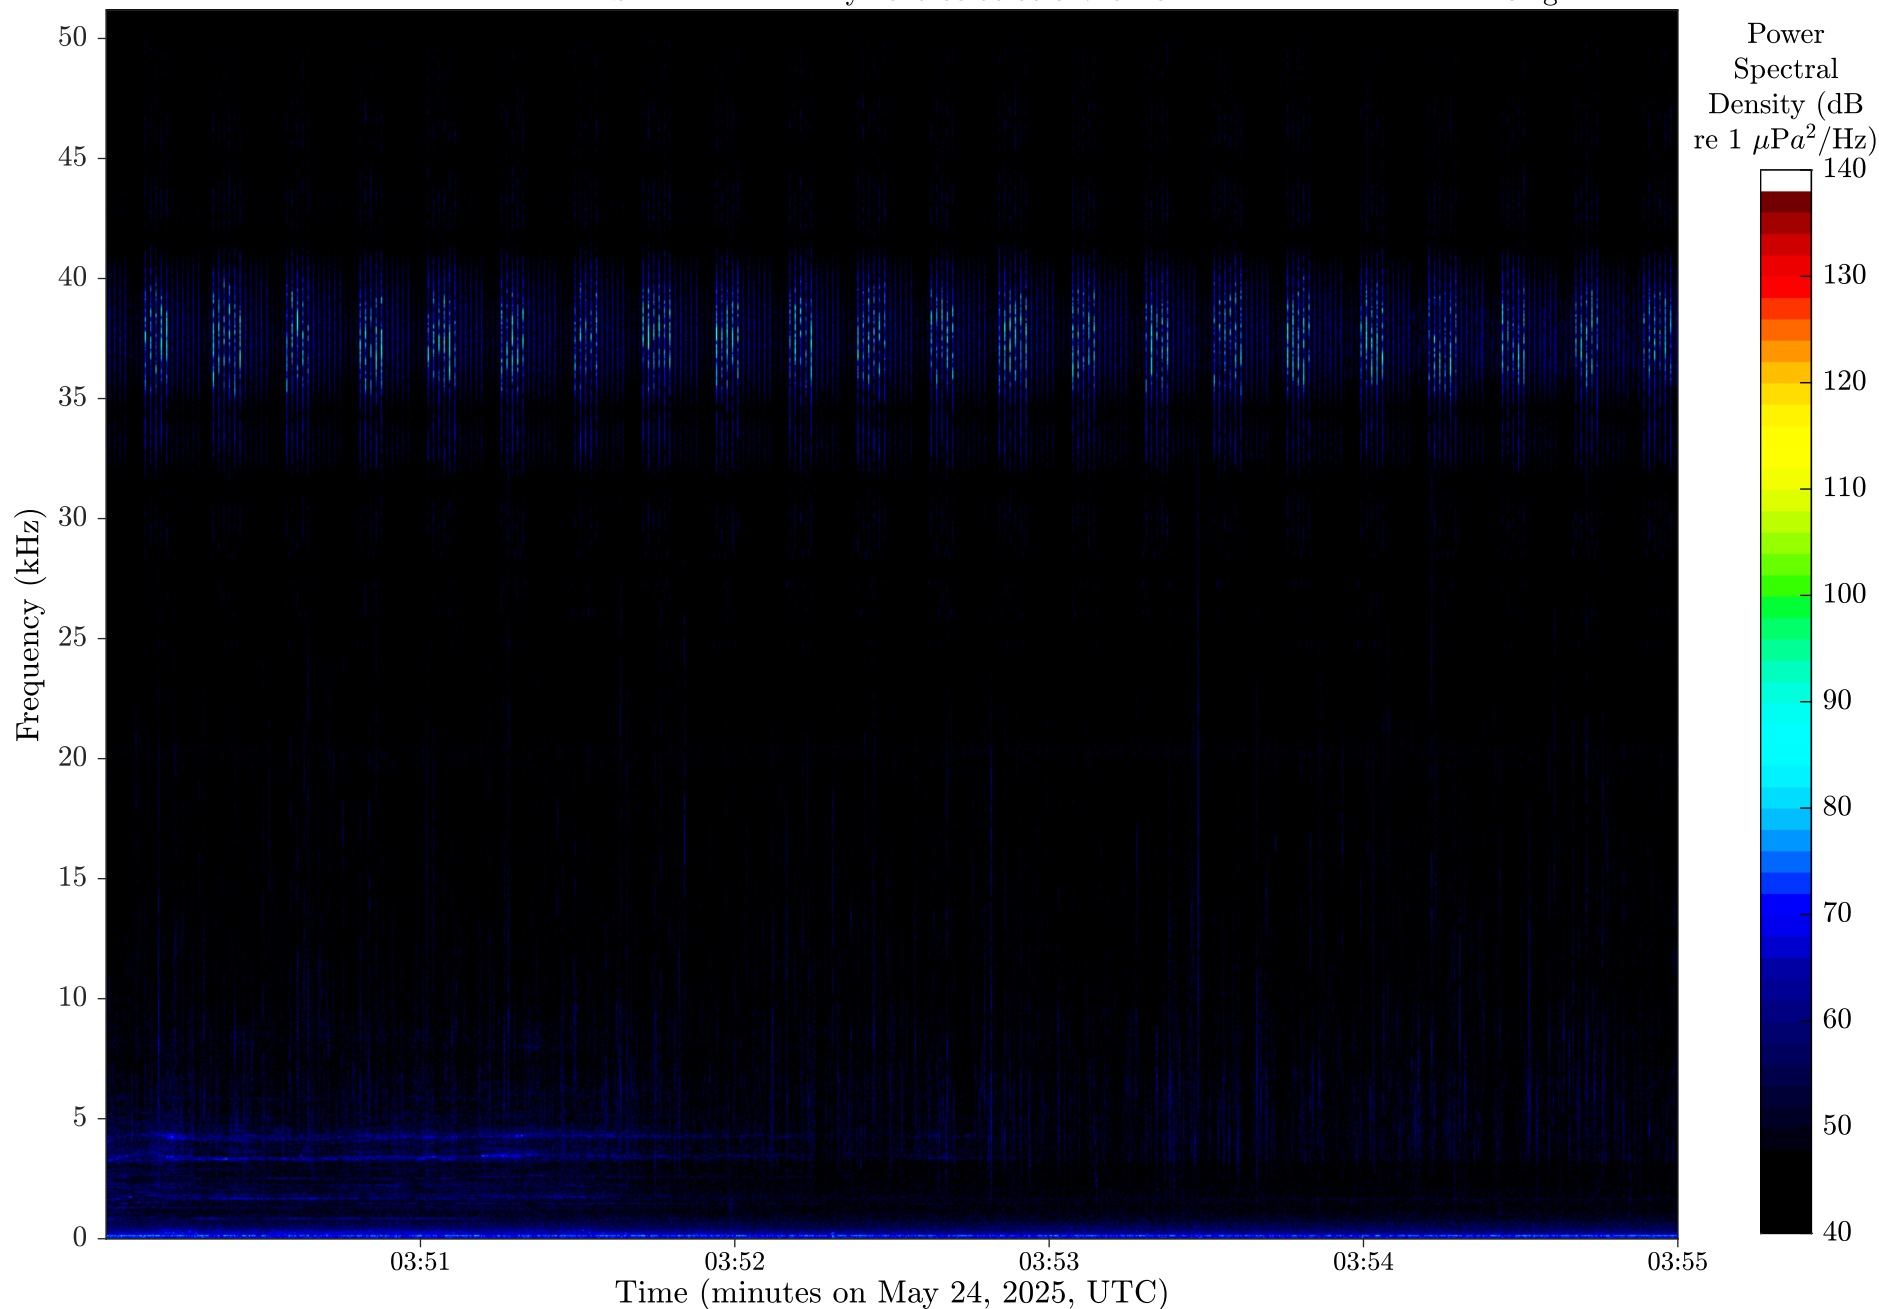


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:17:50 UTC

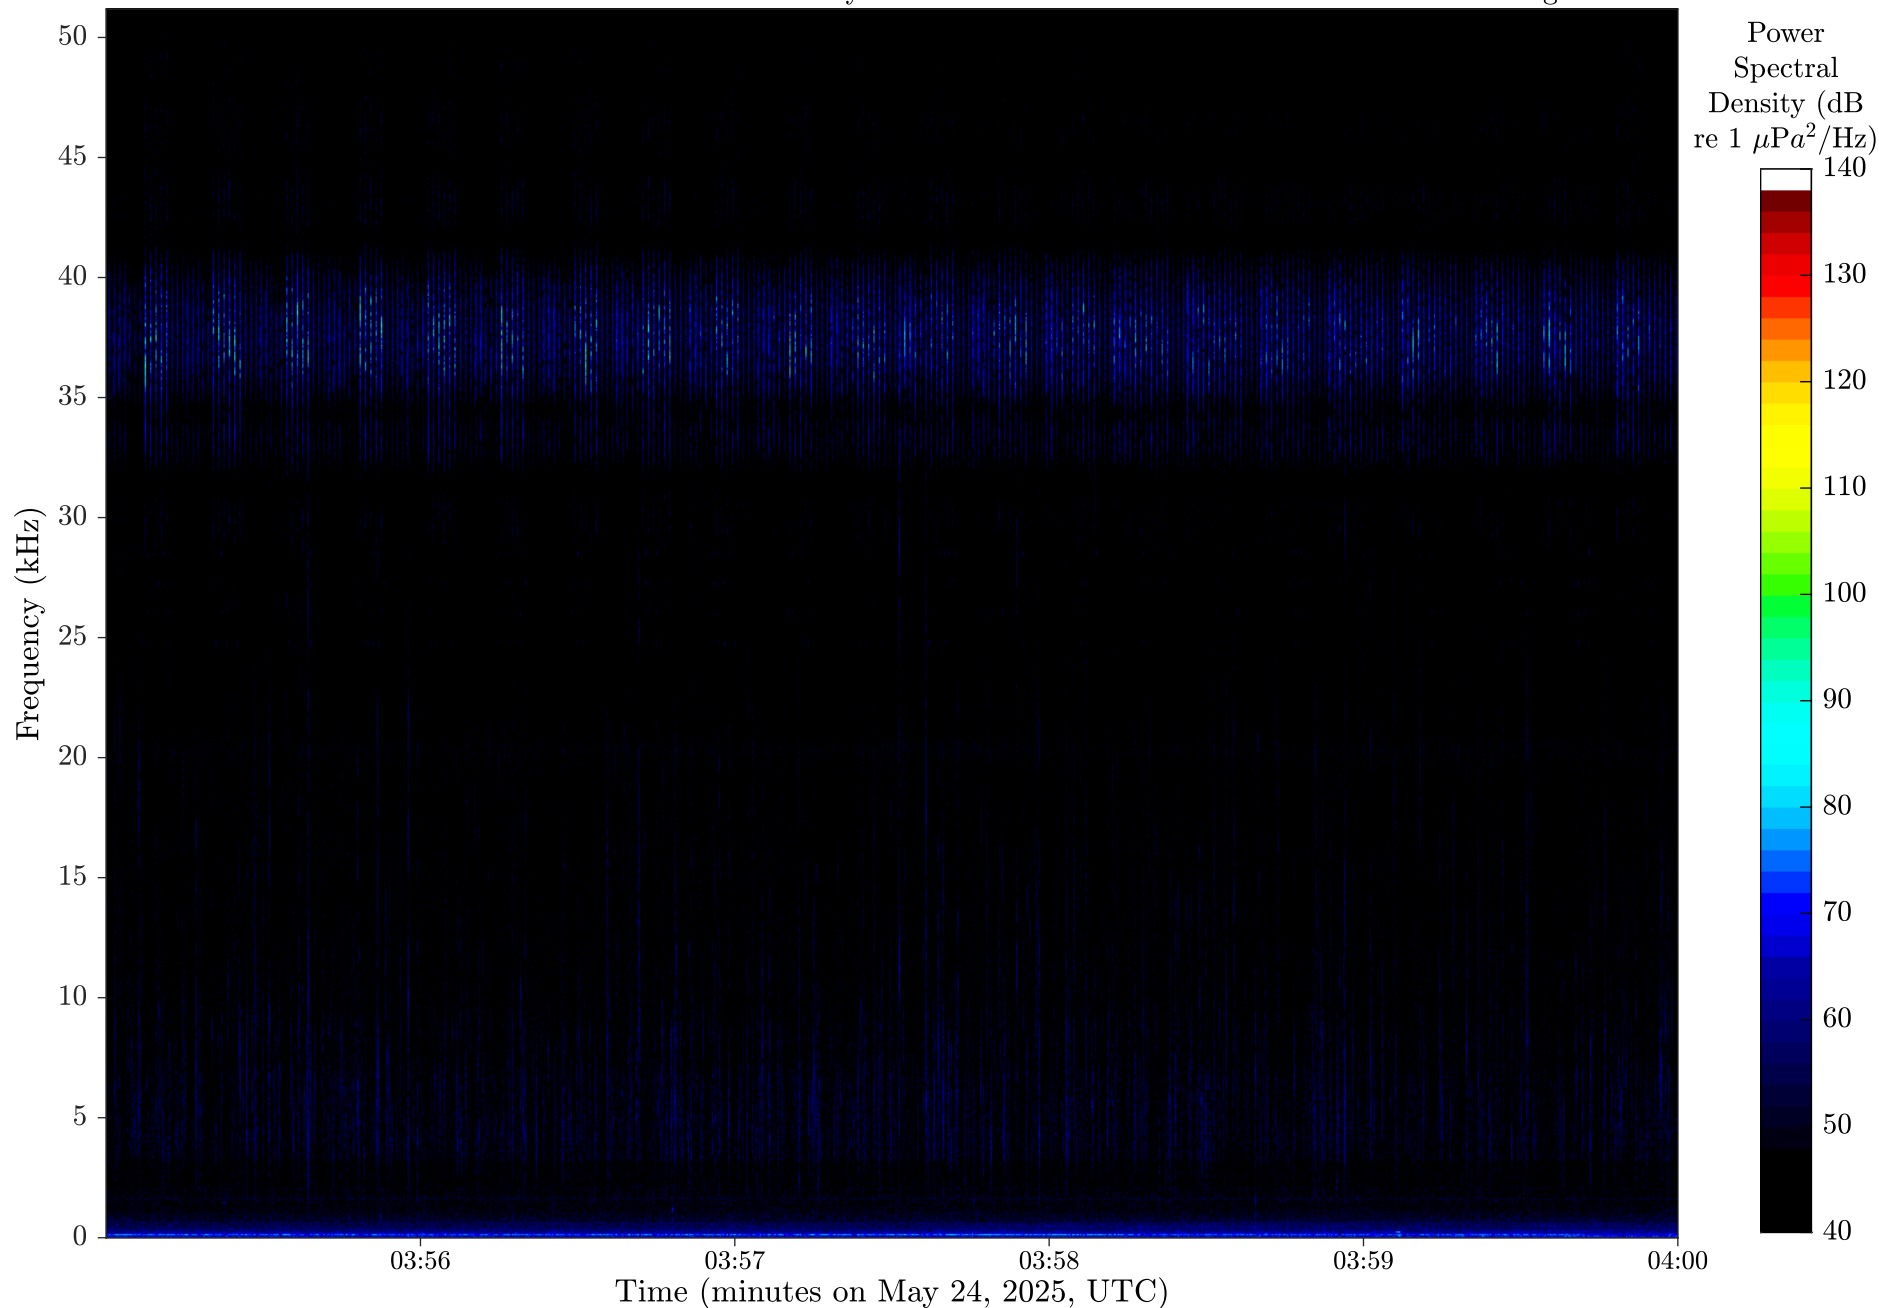

Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:17:58 UTC

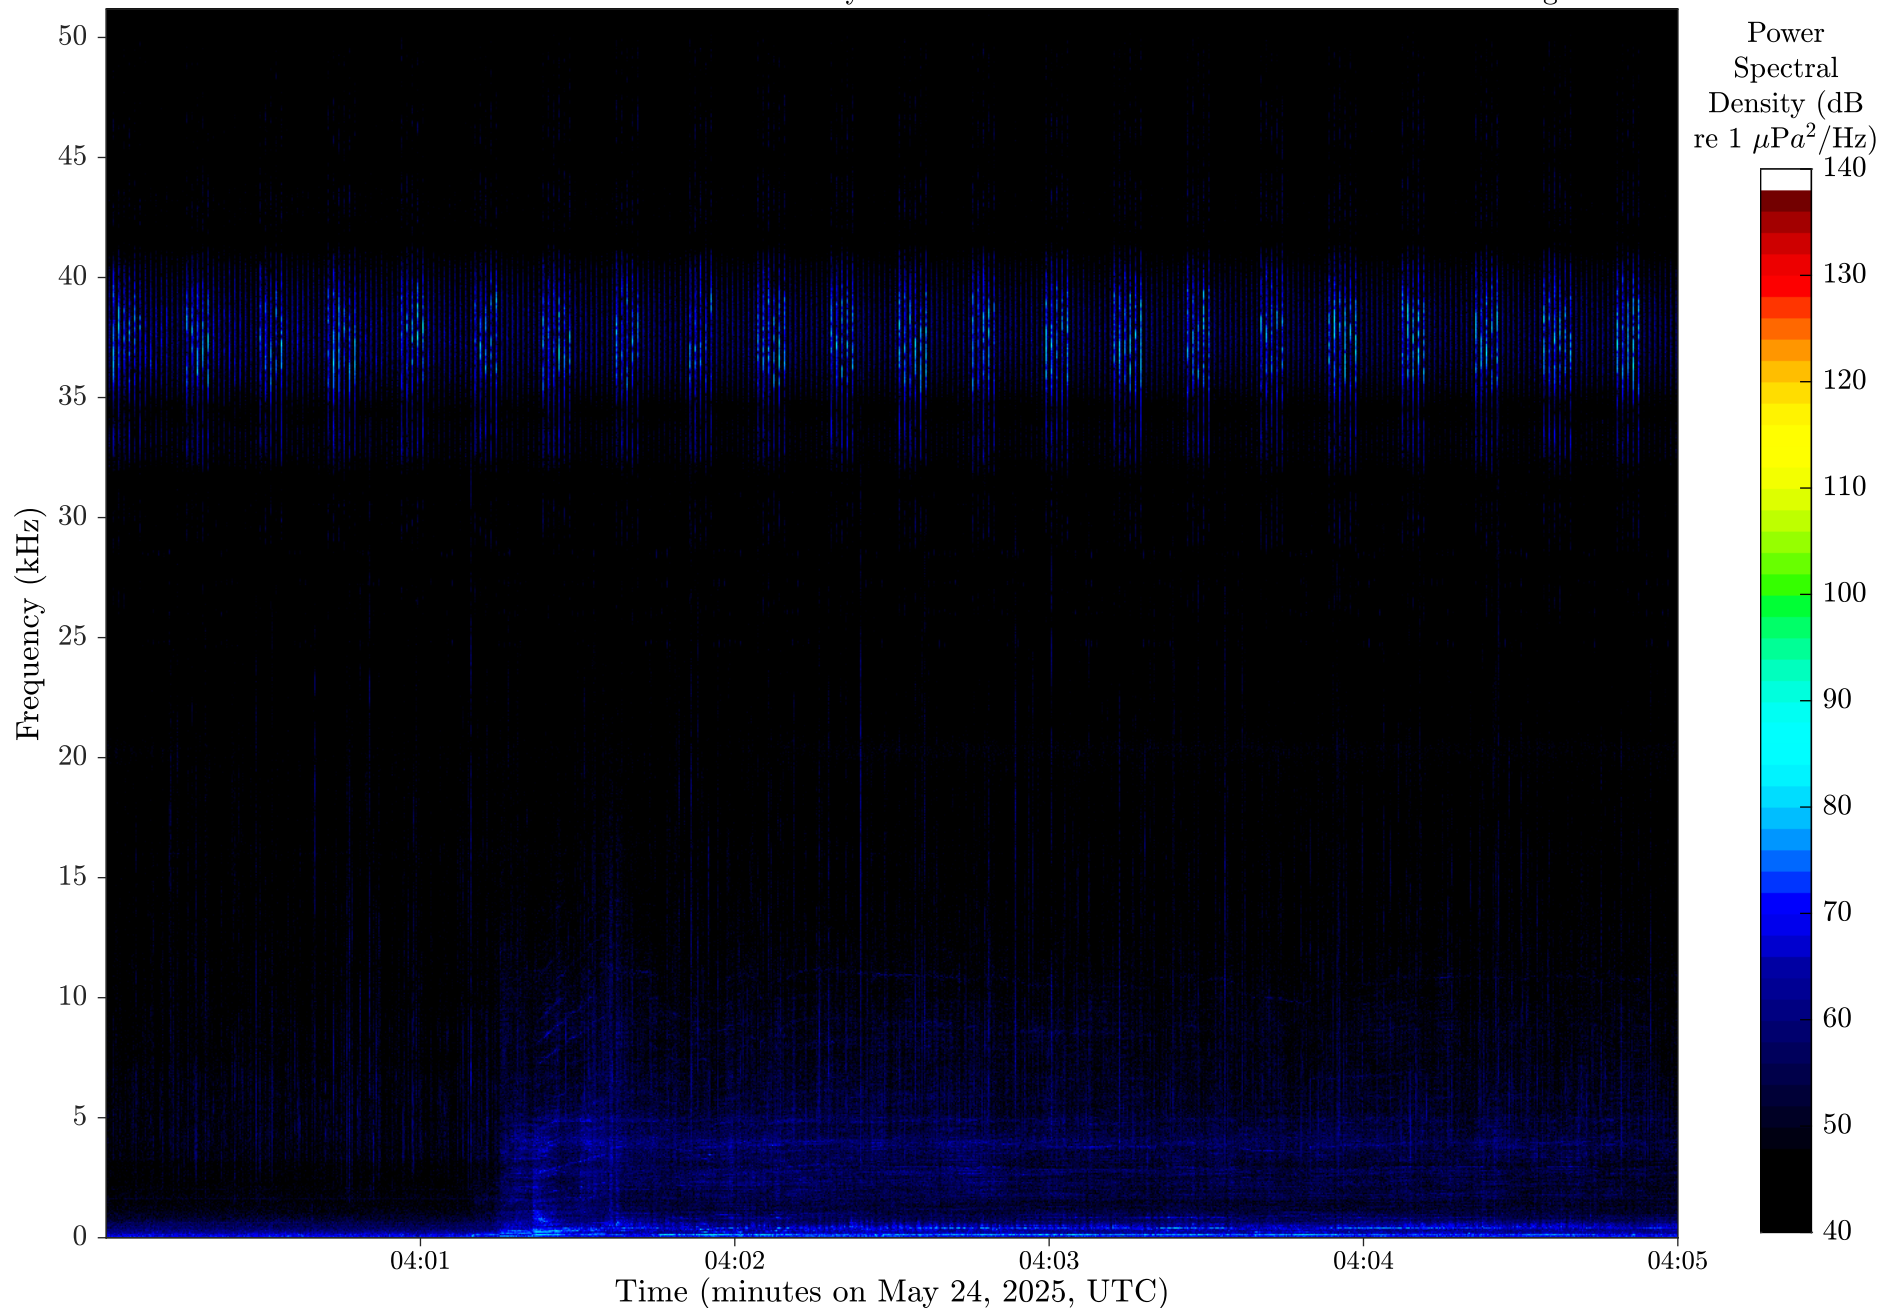


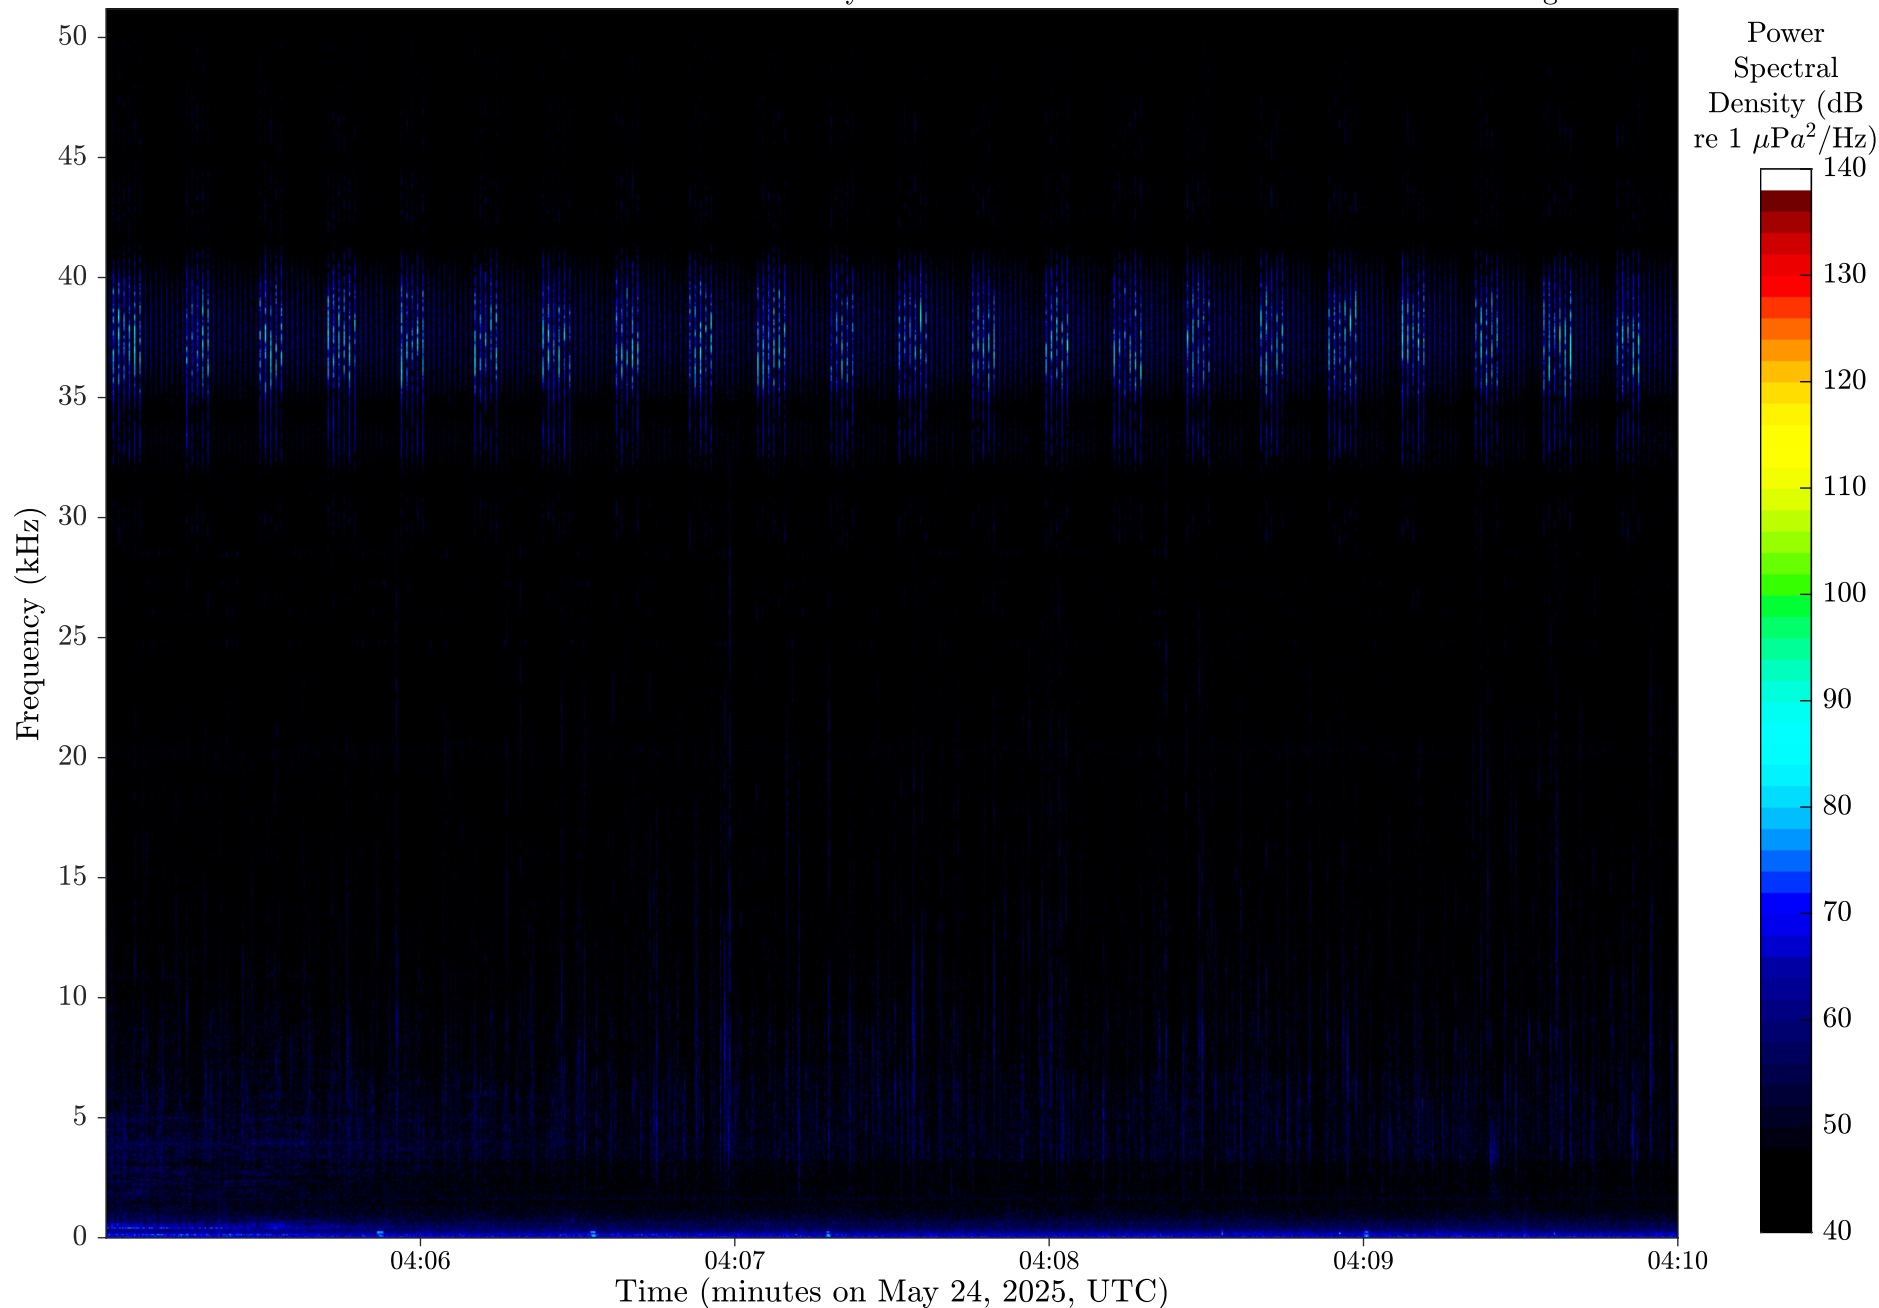



Comments: 34.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:18:12 UTC

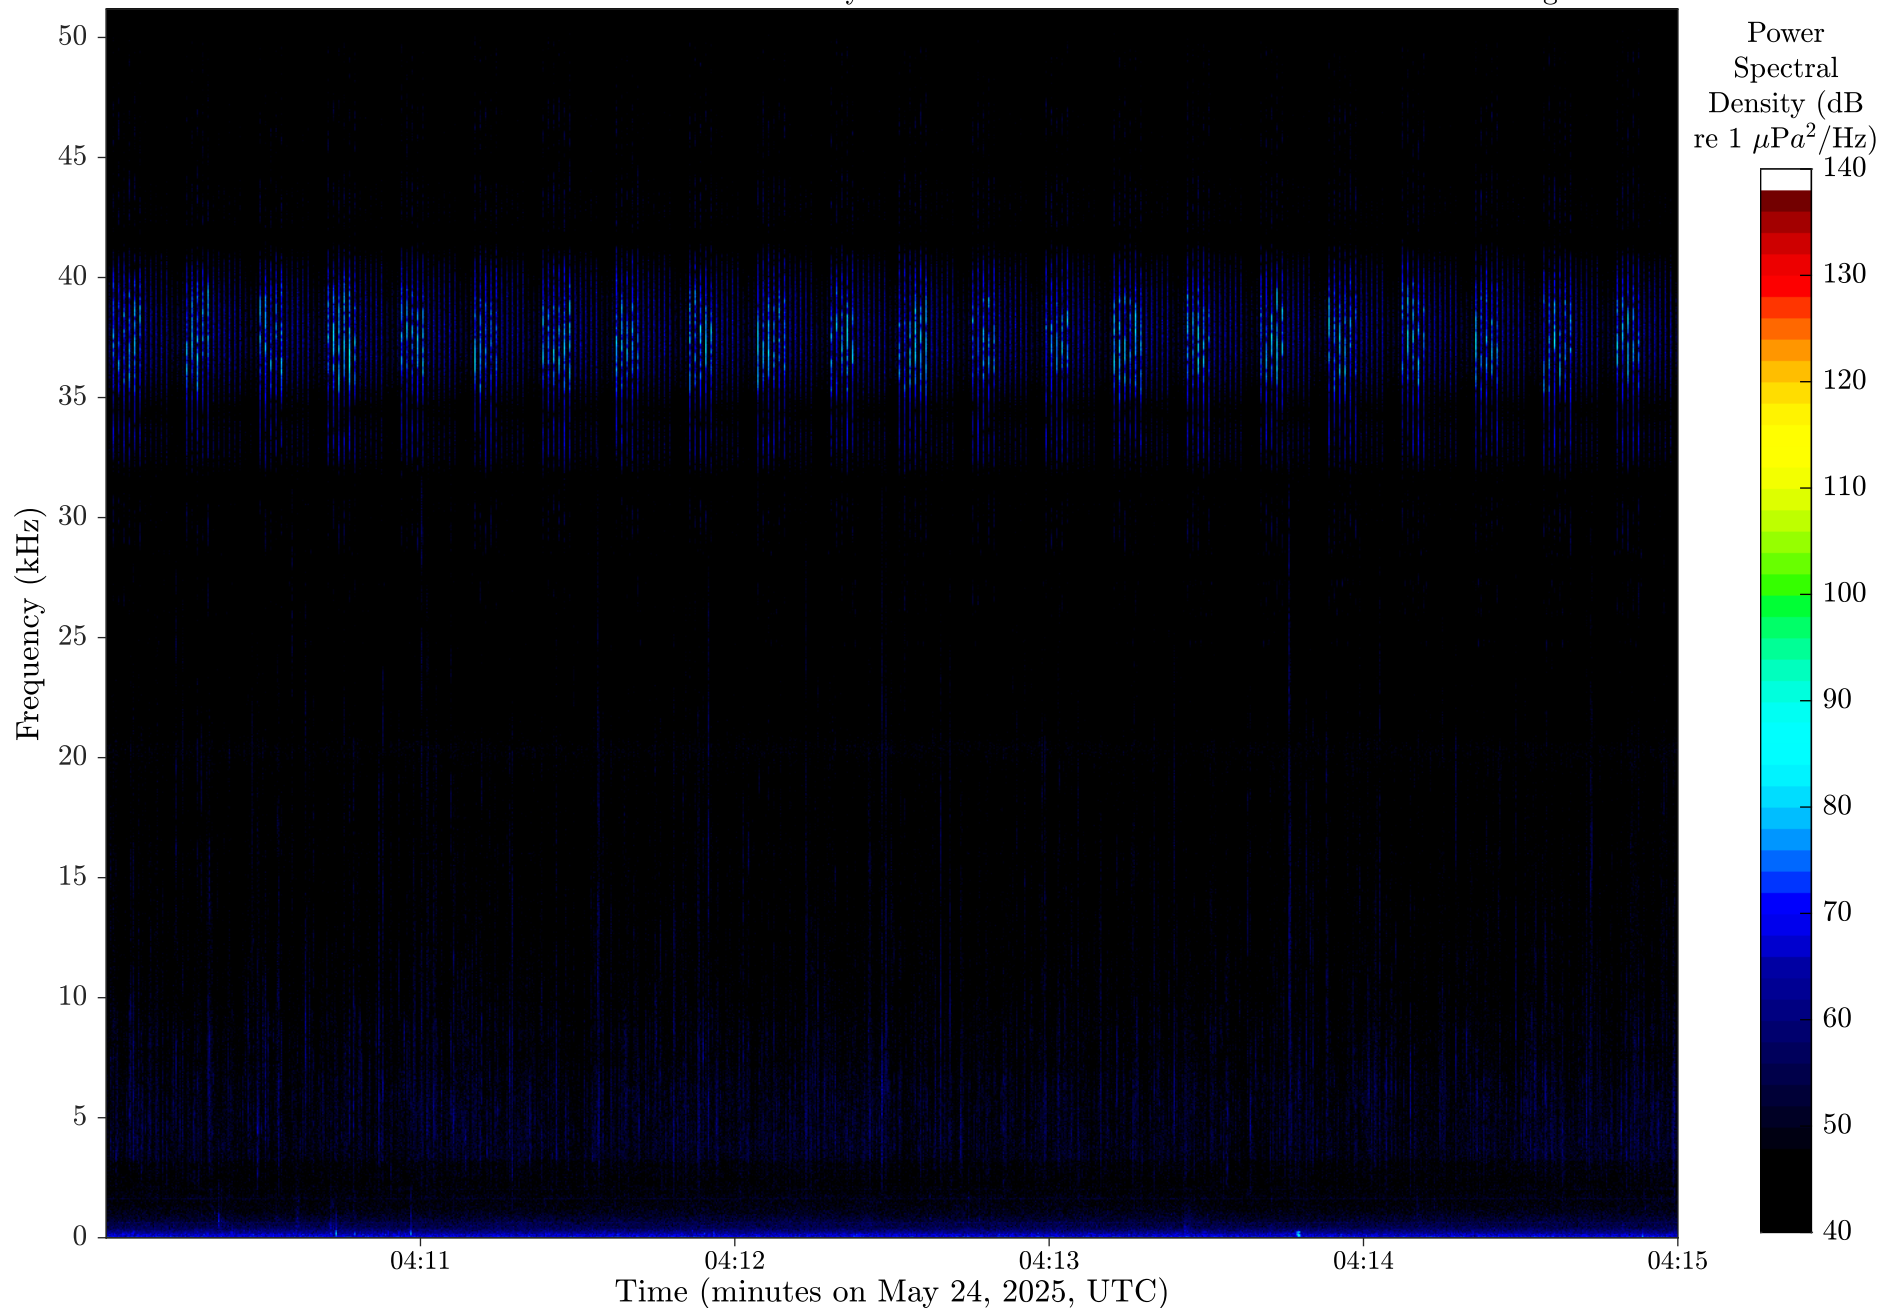

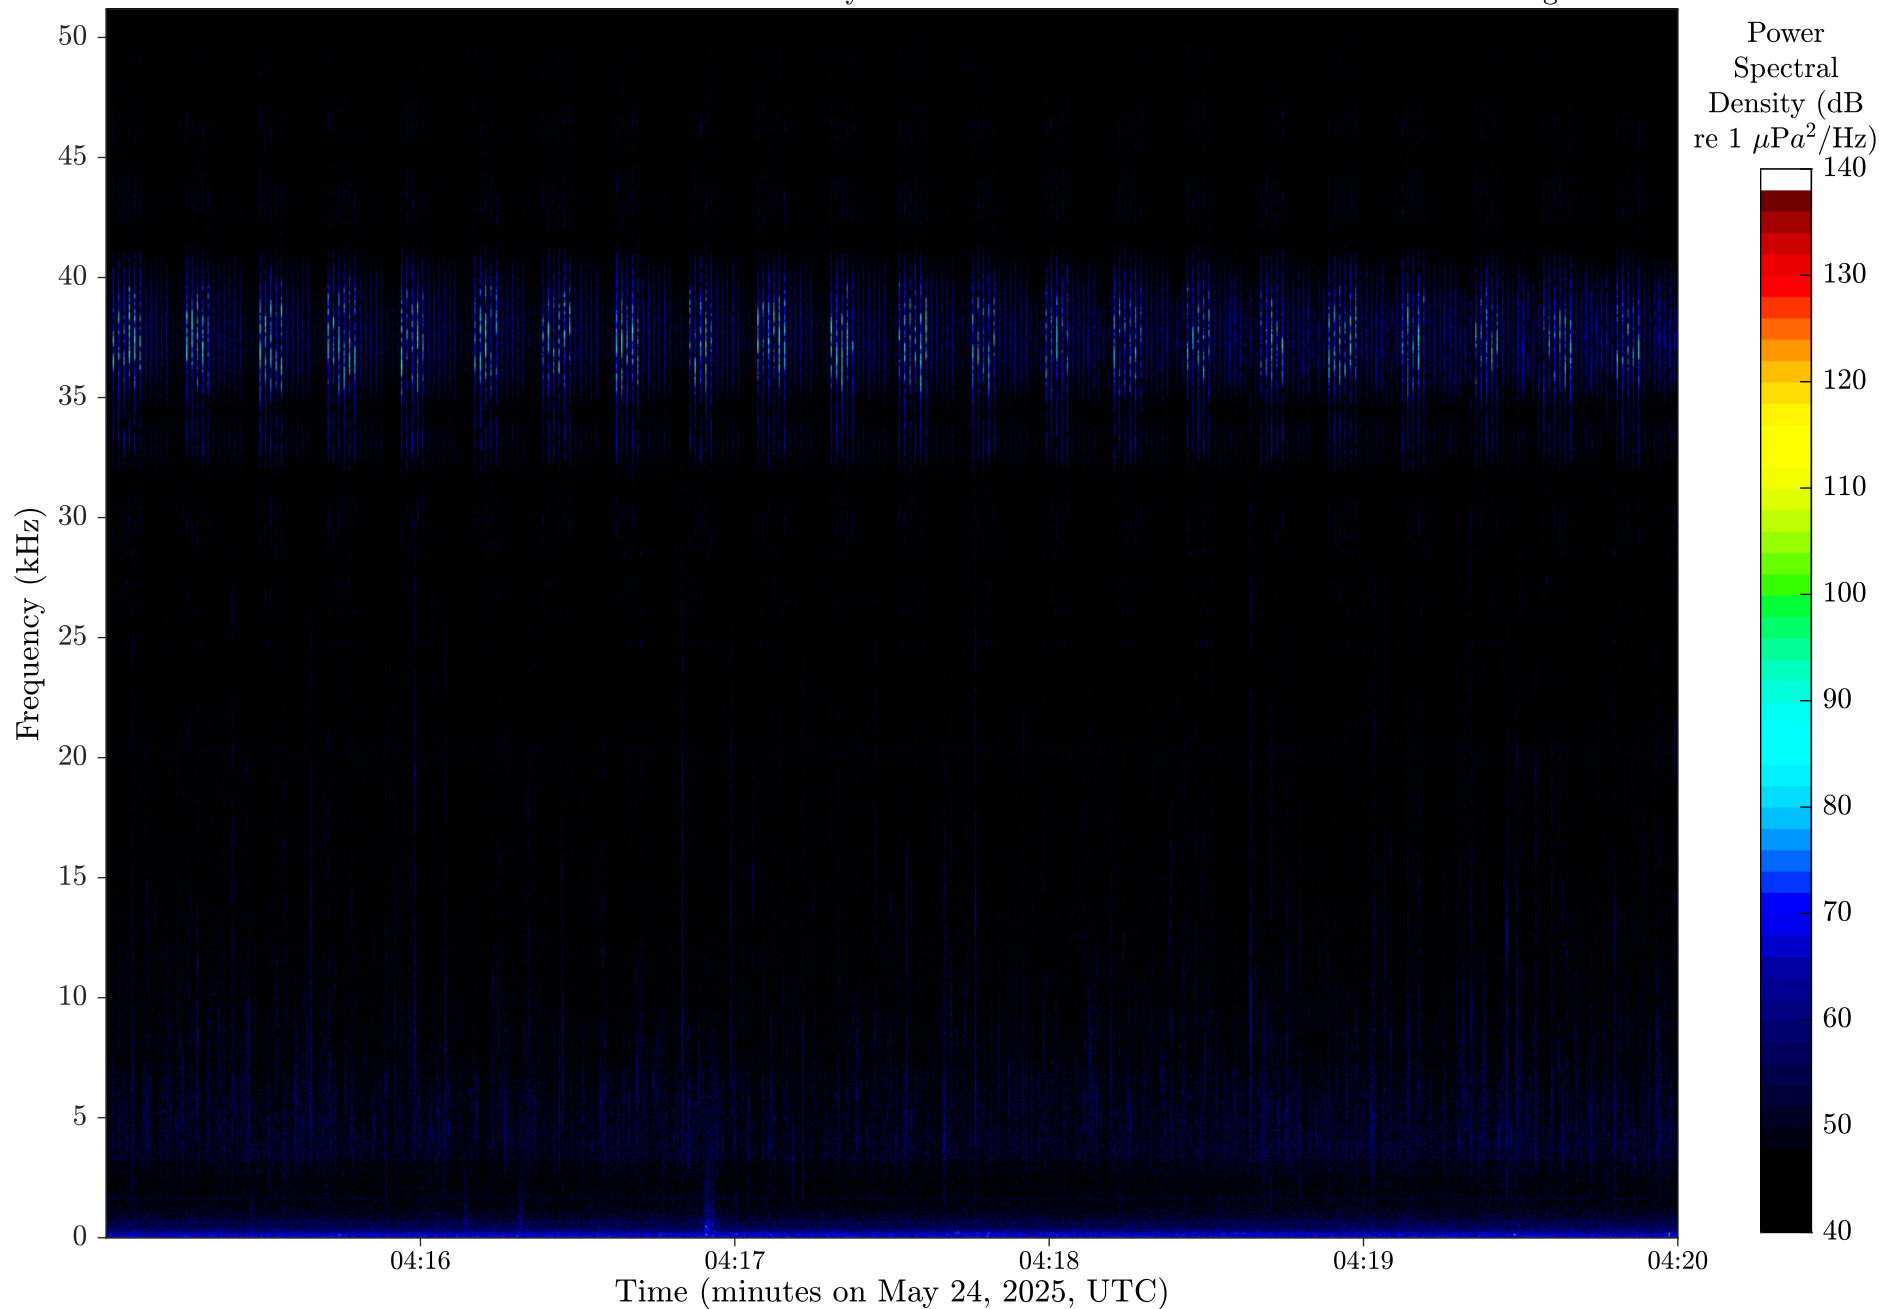


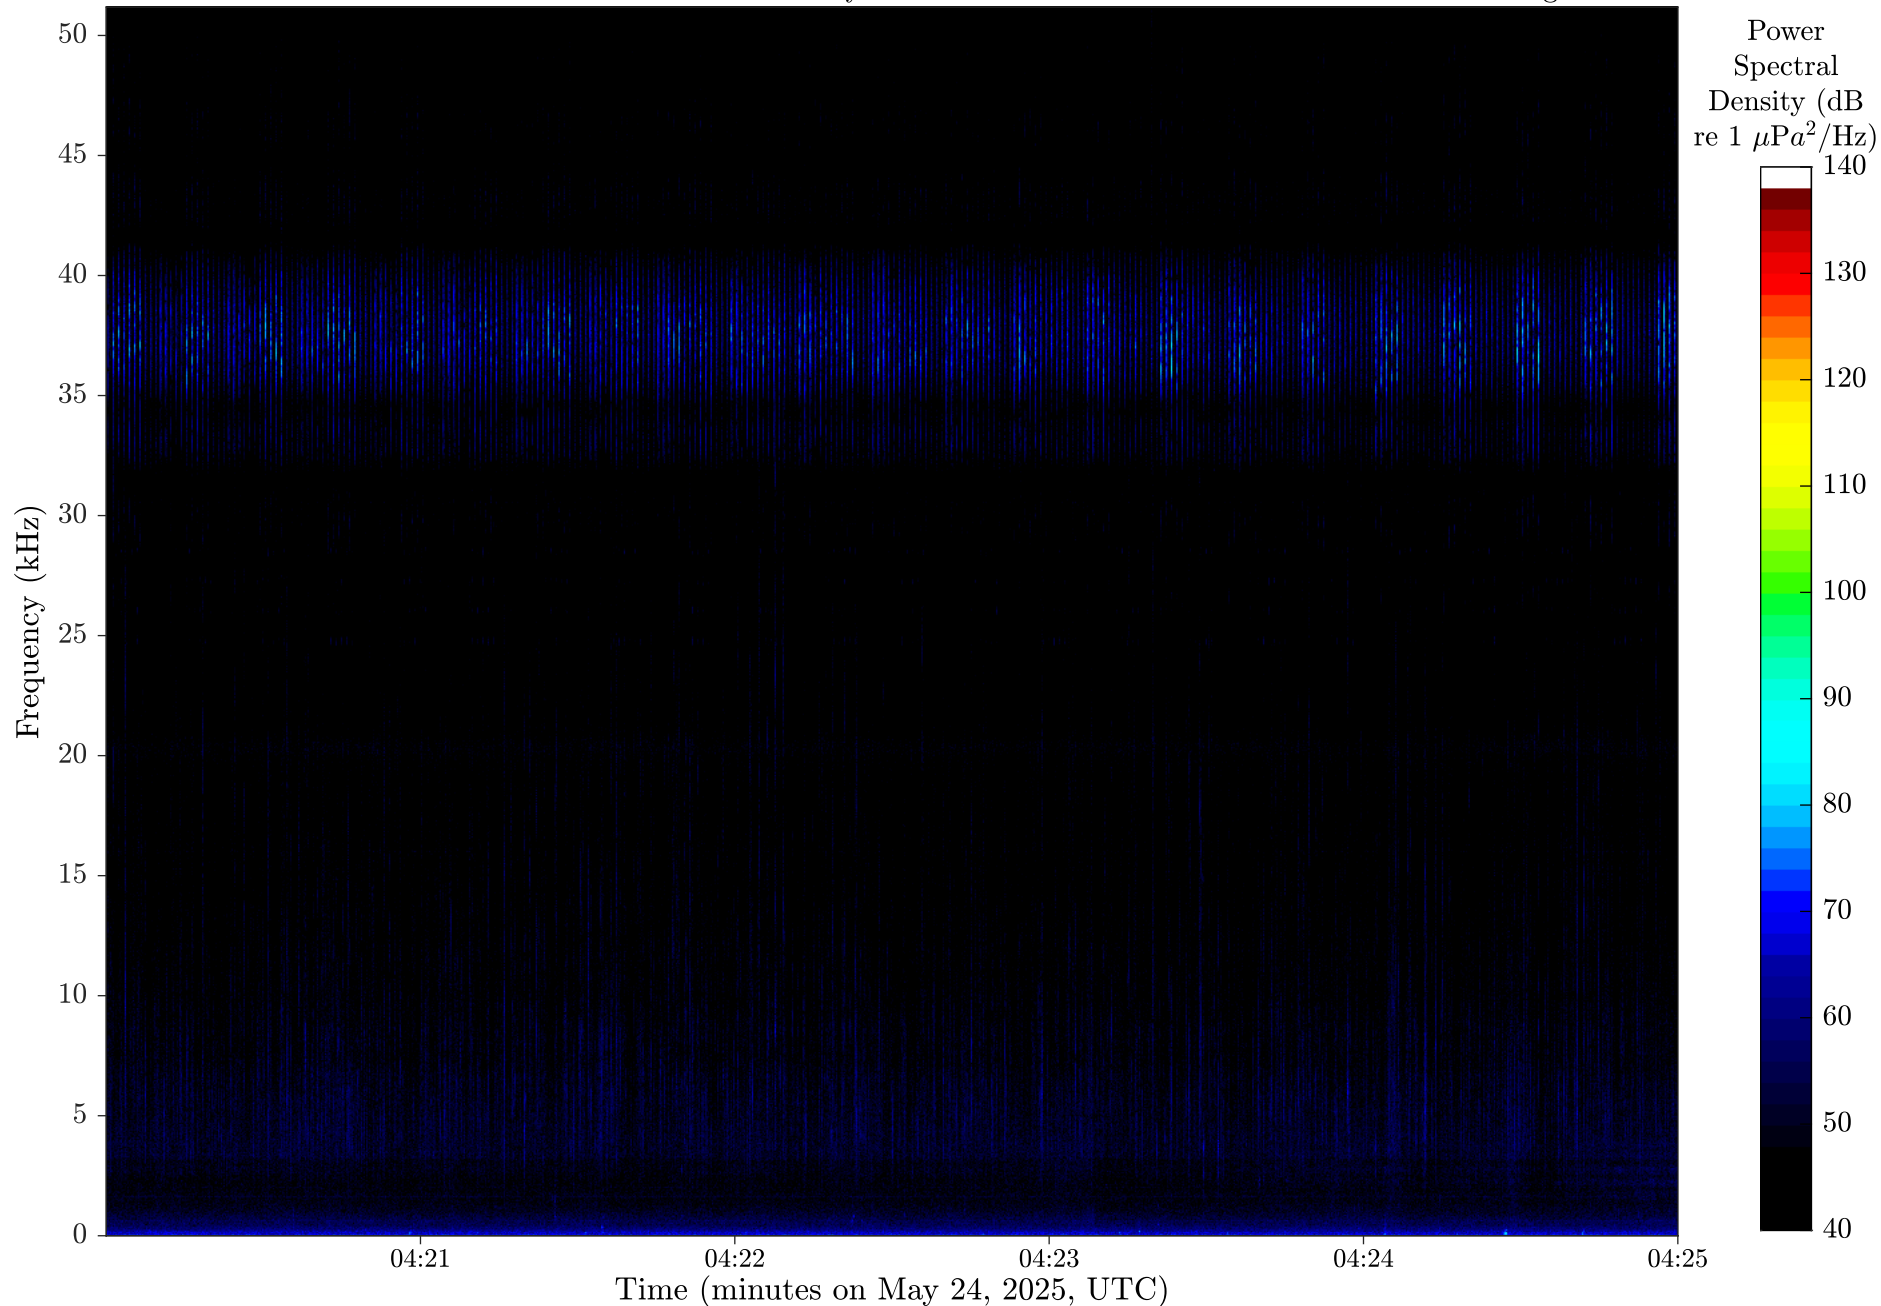

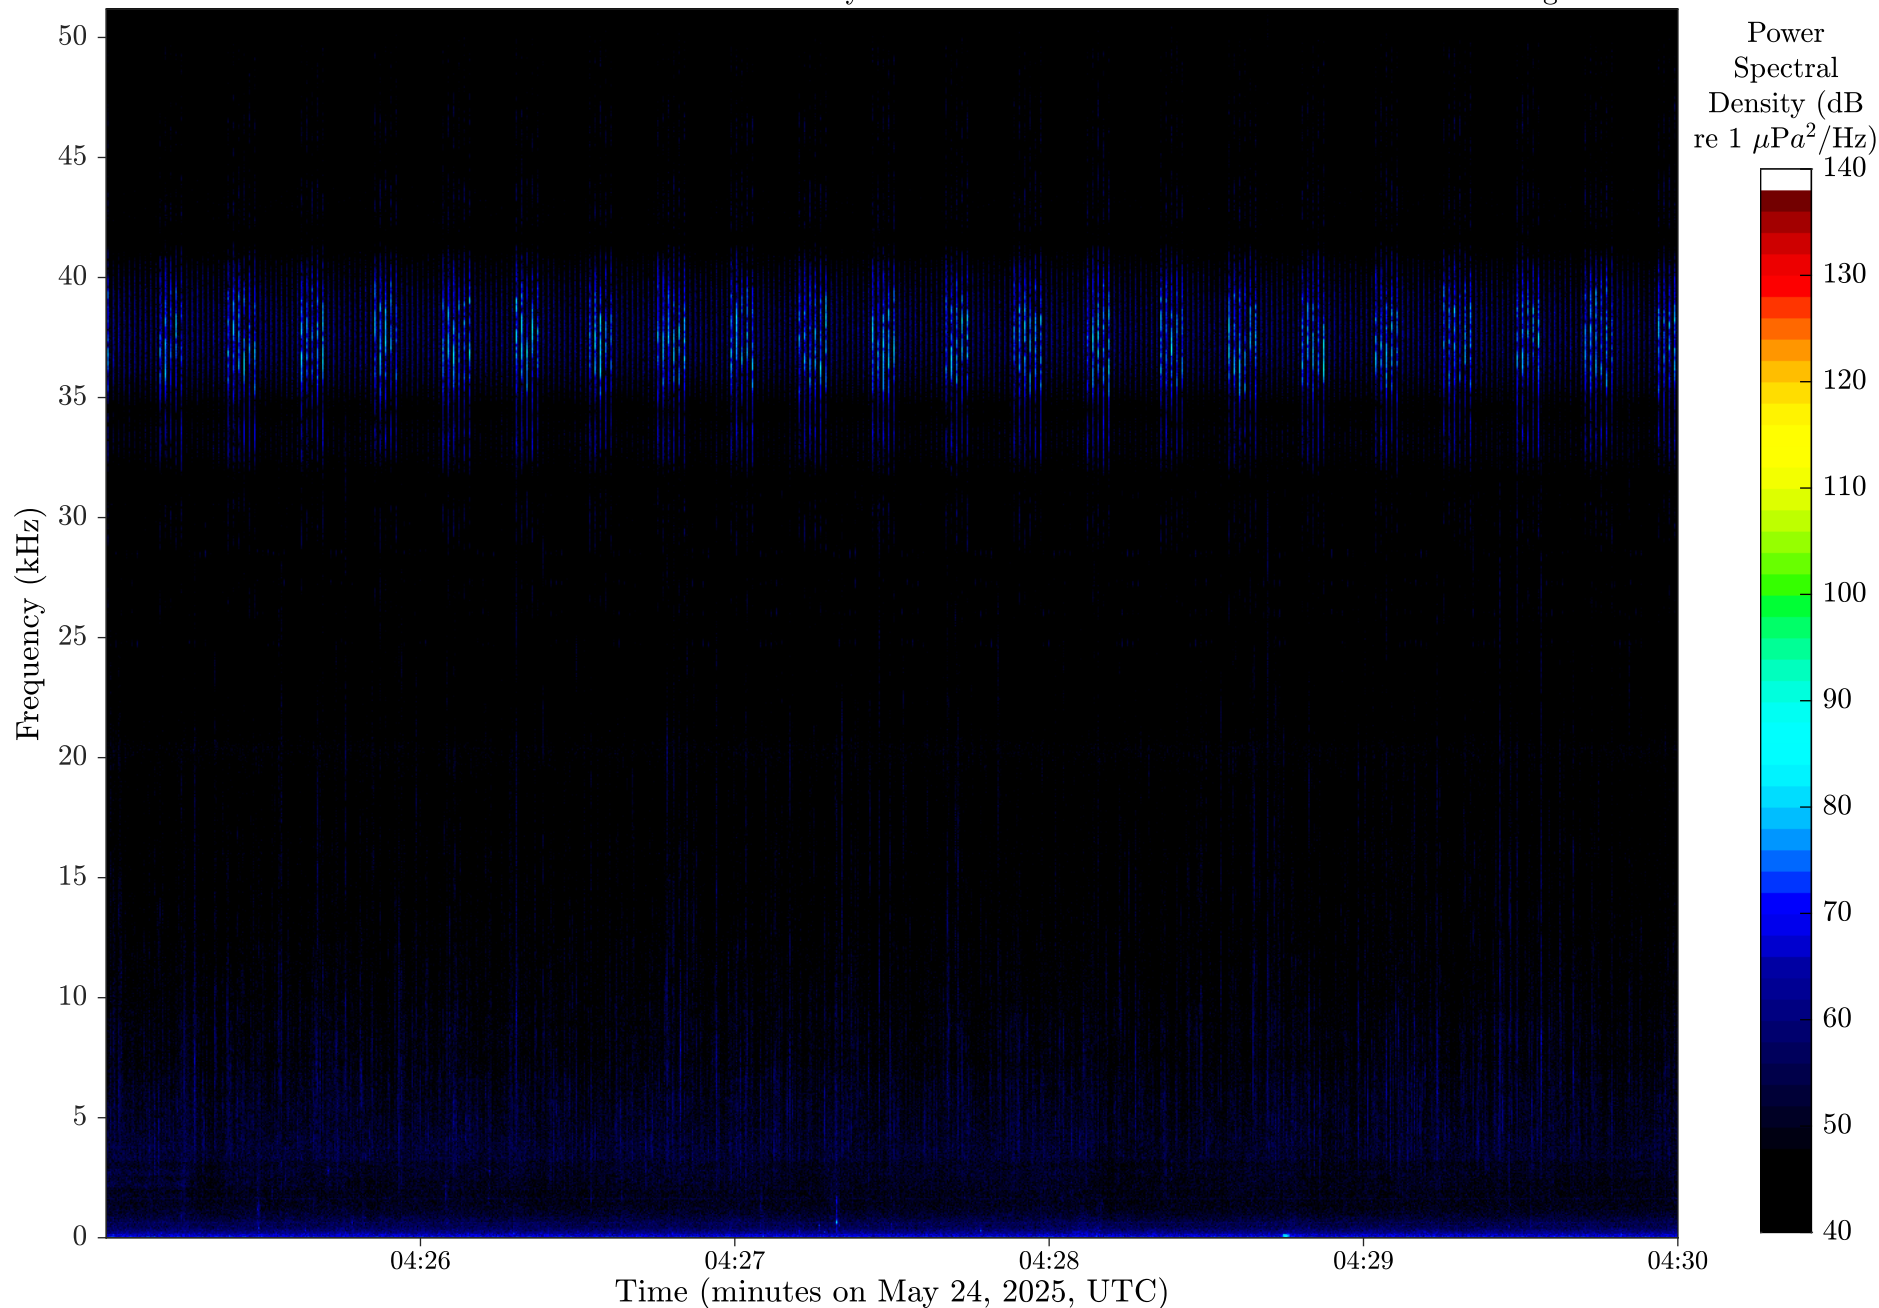


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:18:42 UTC

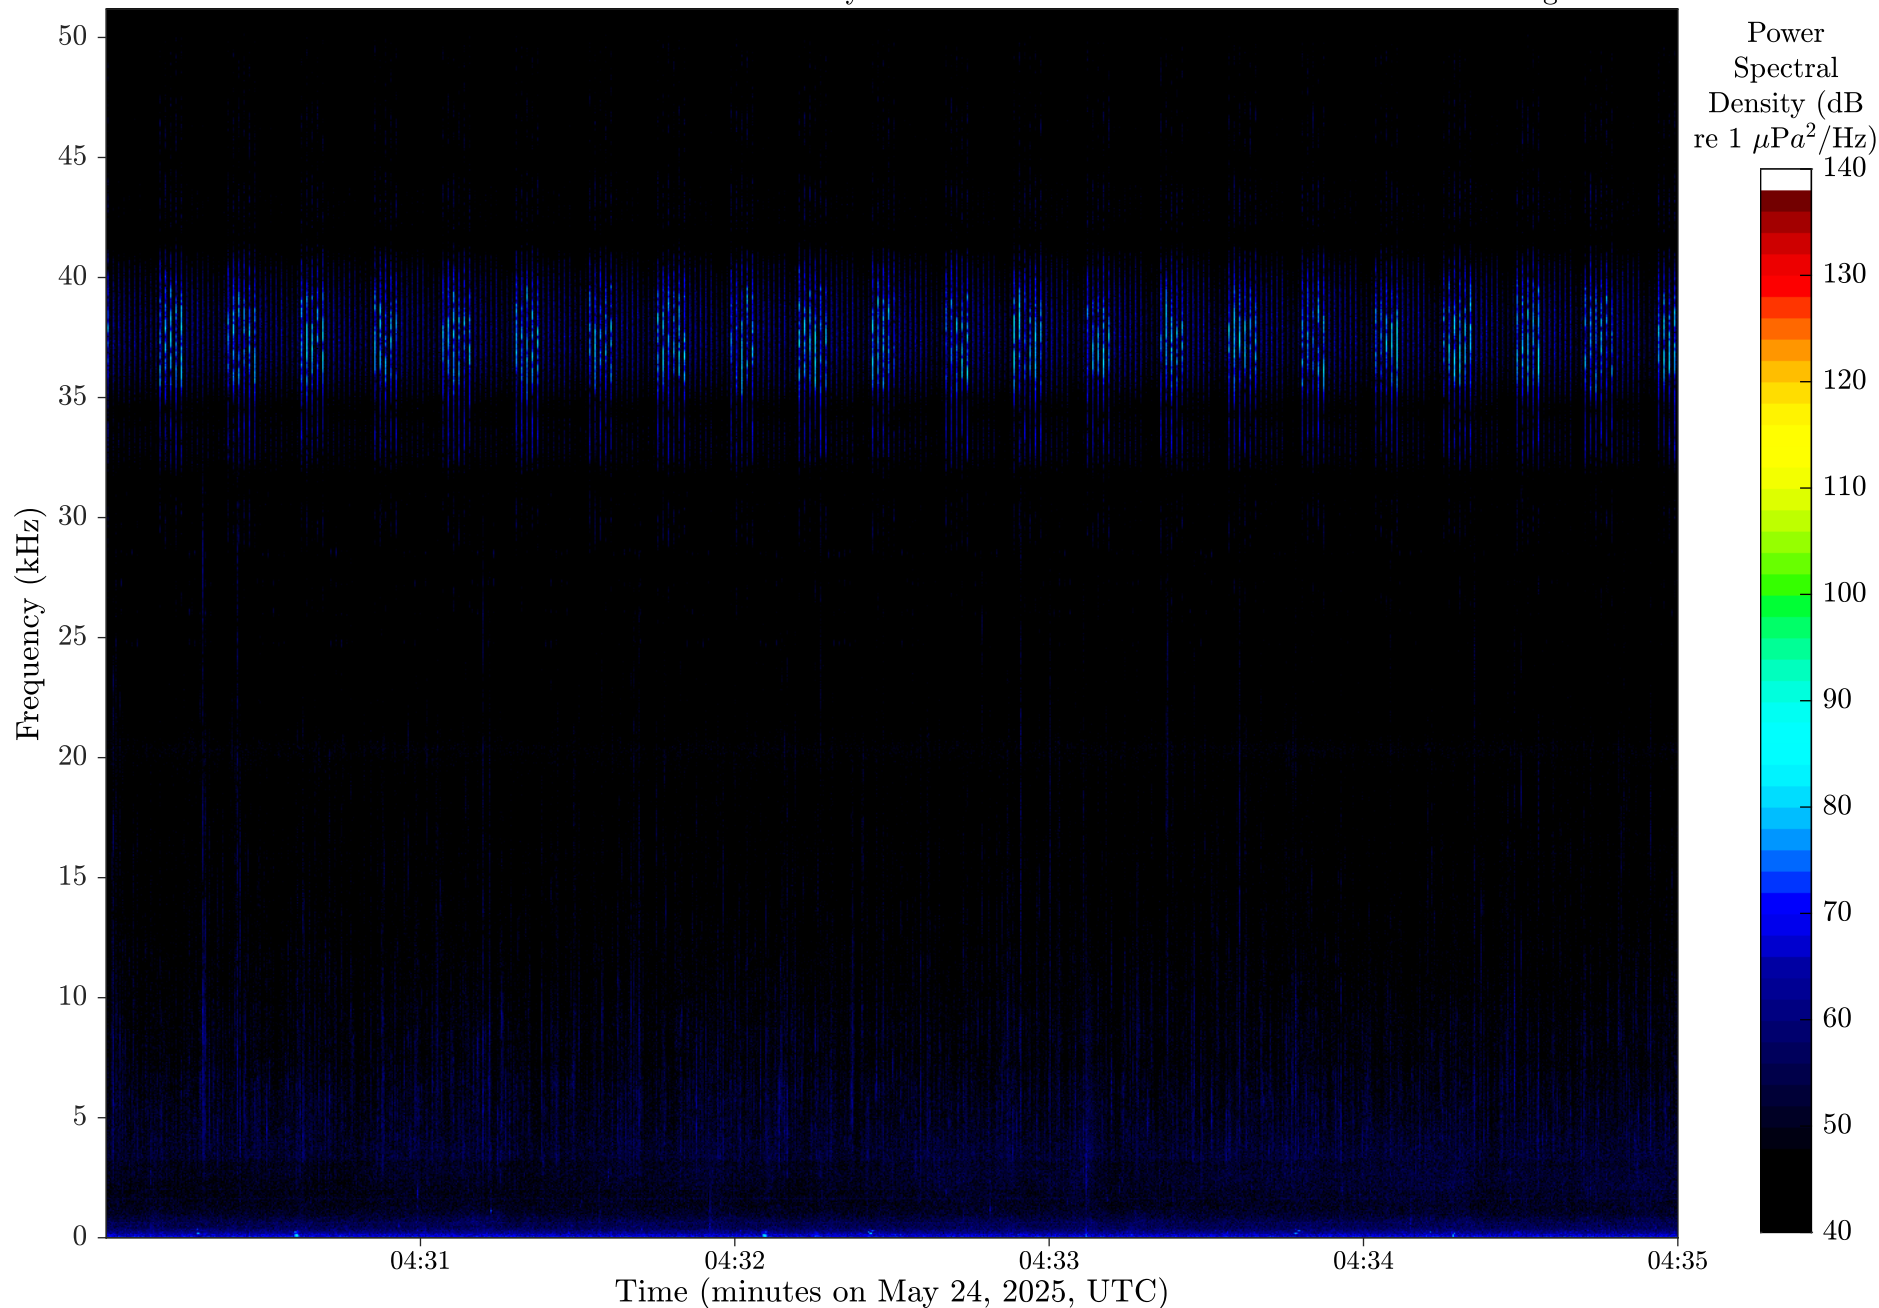


Comments: 34.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:18:50 UTC

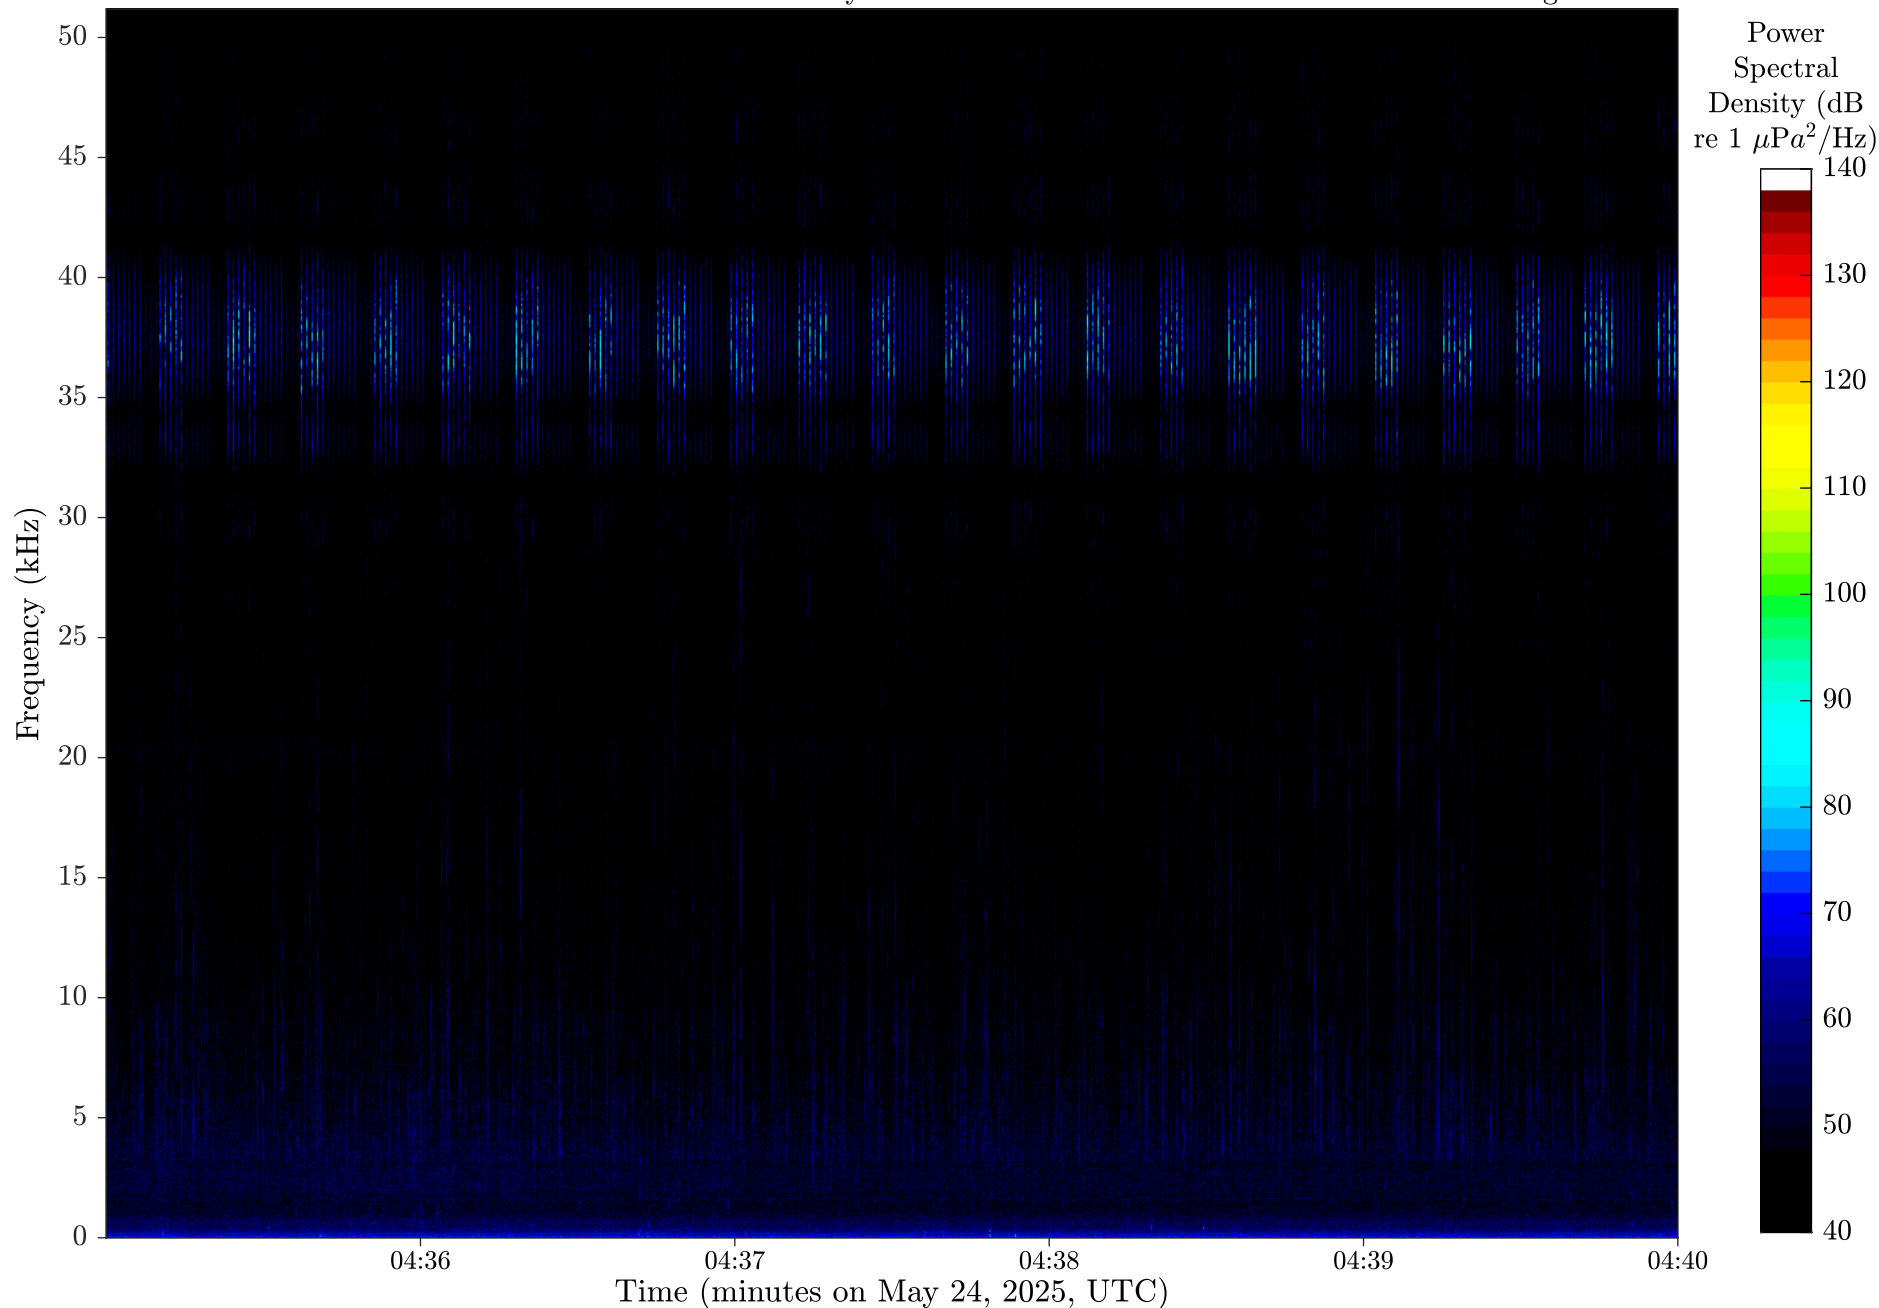


Comments: 34.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:18:57 UTC

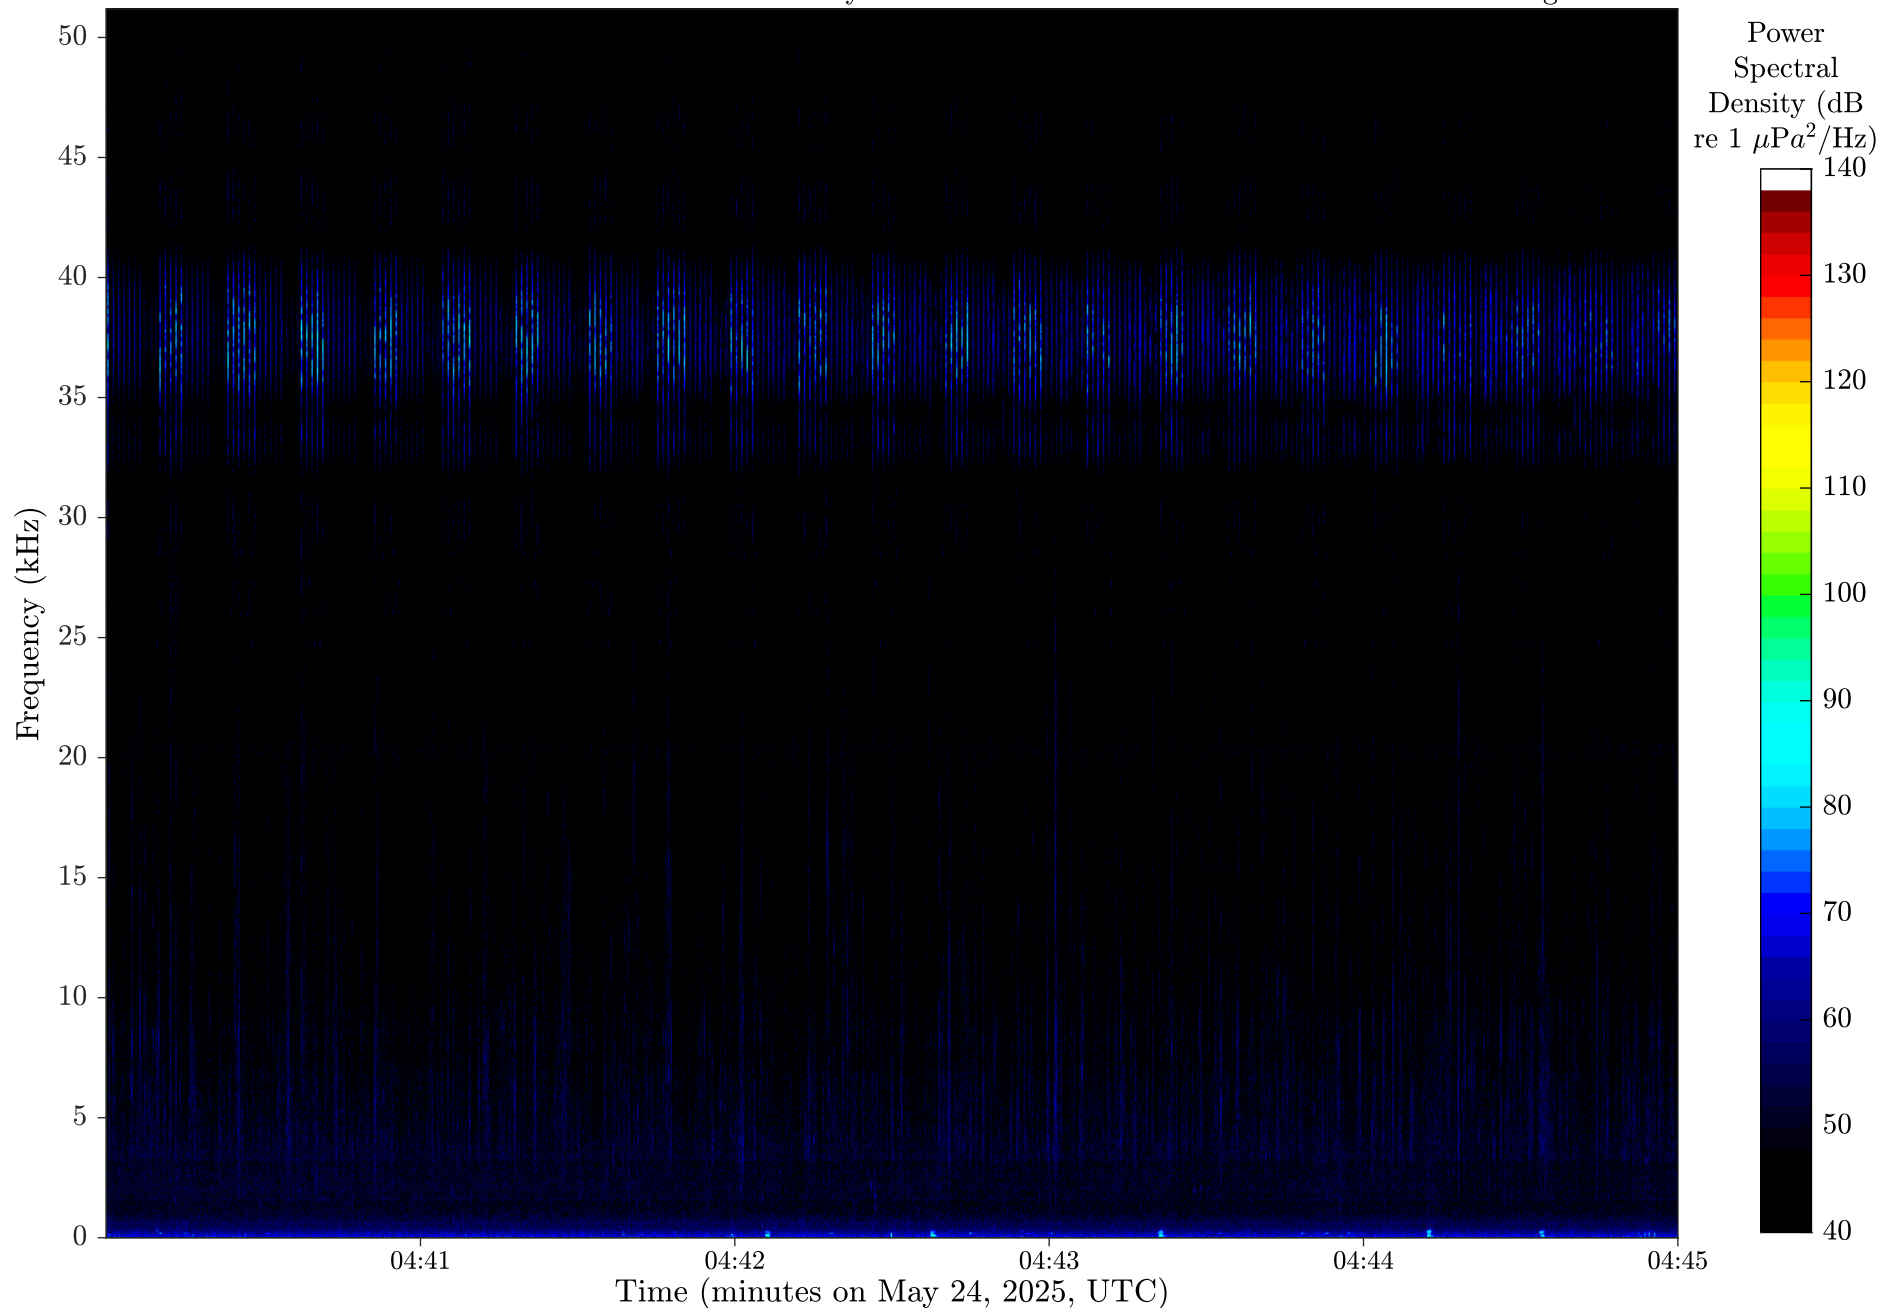


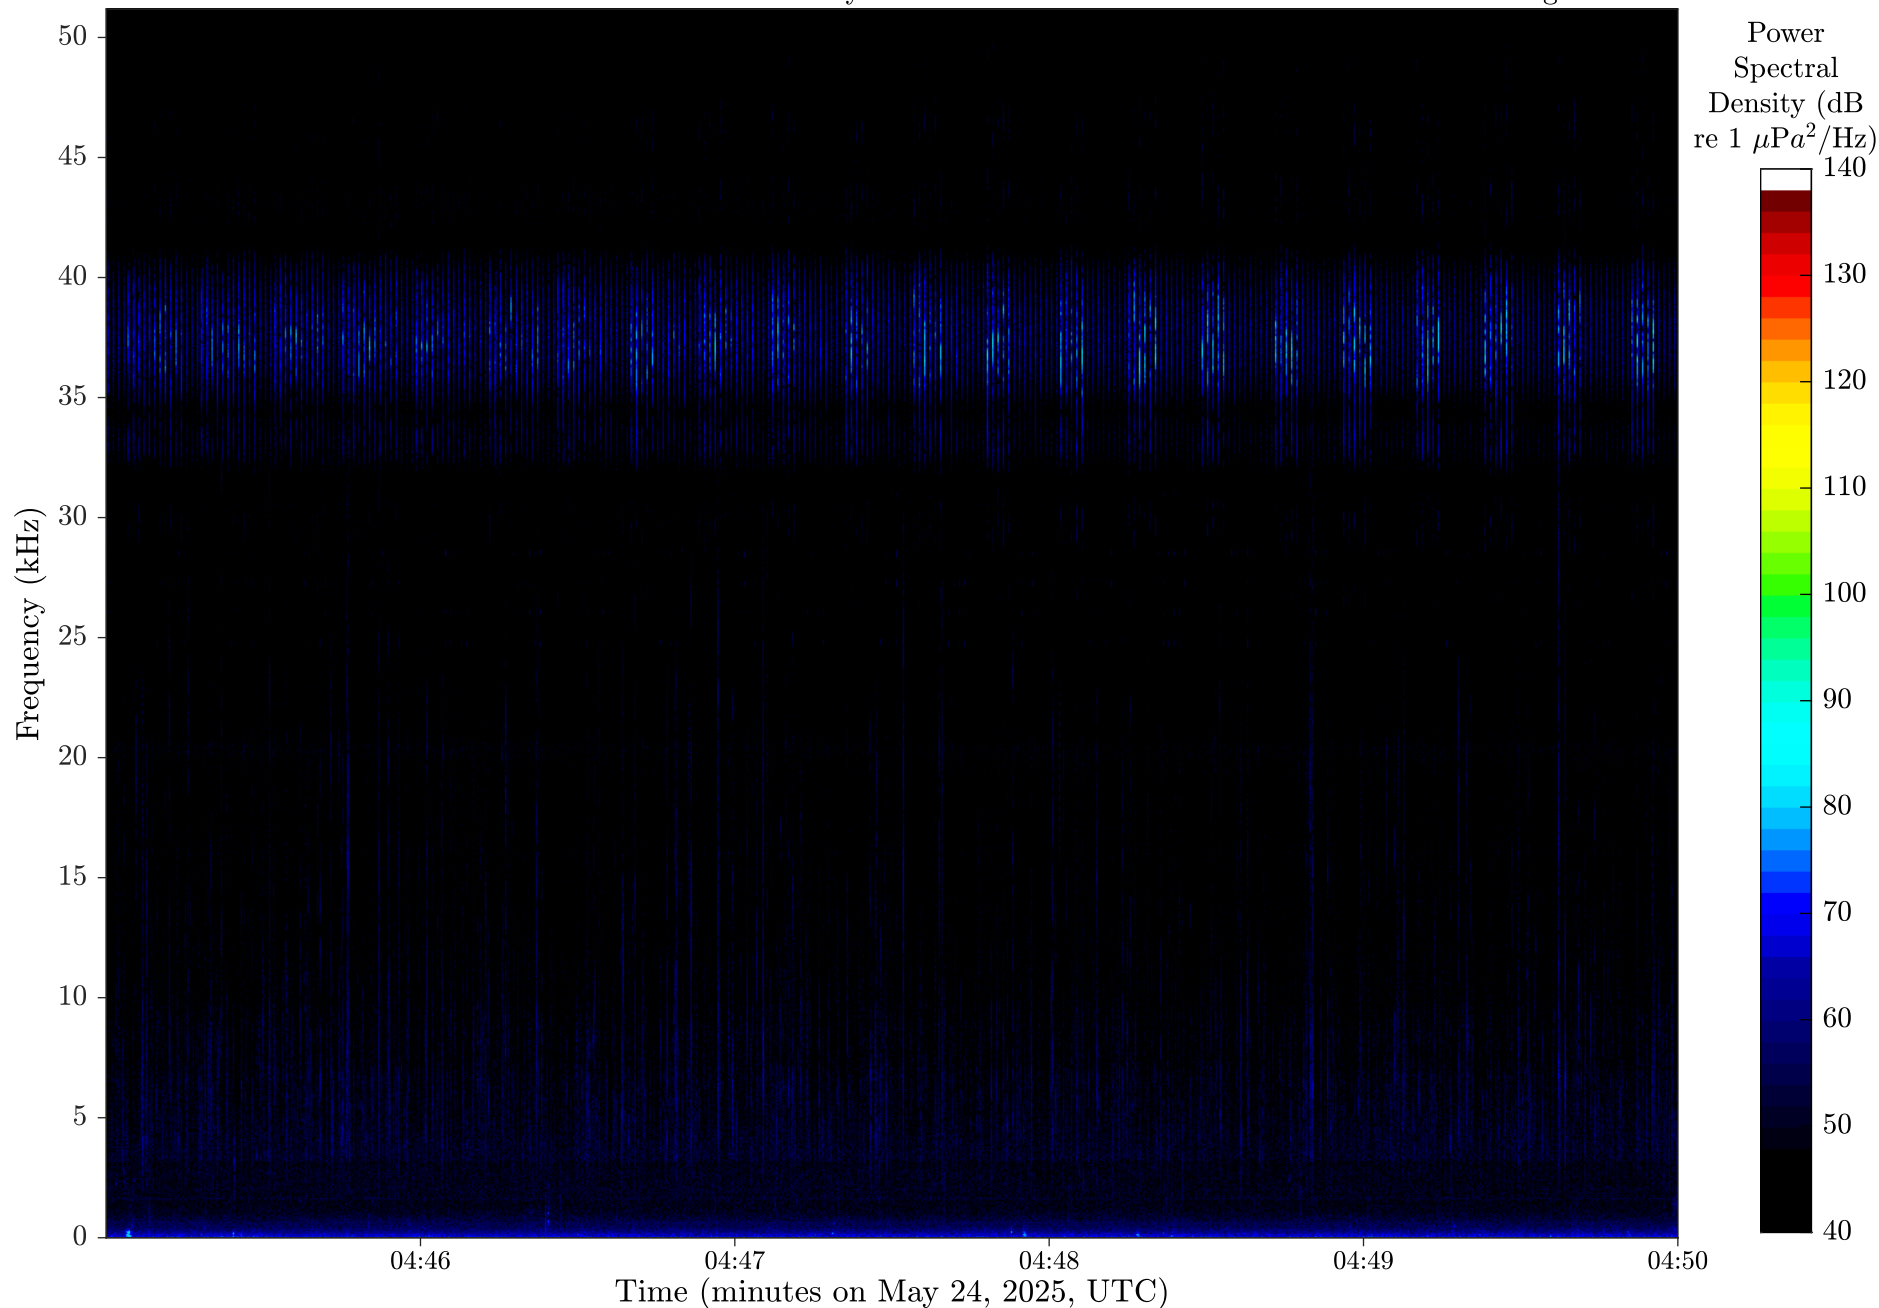

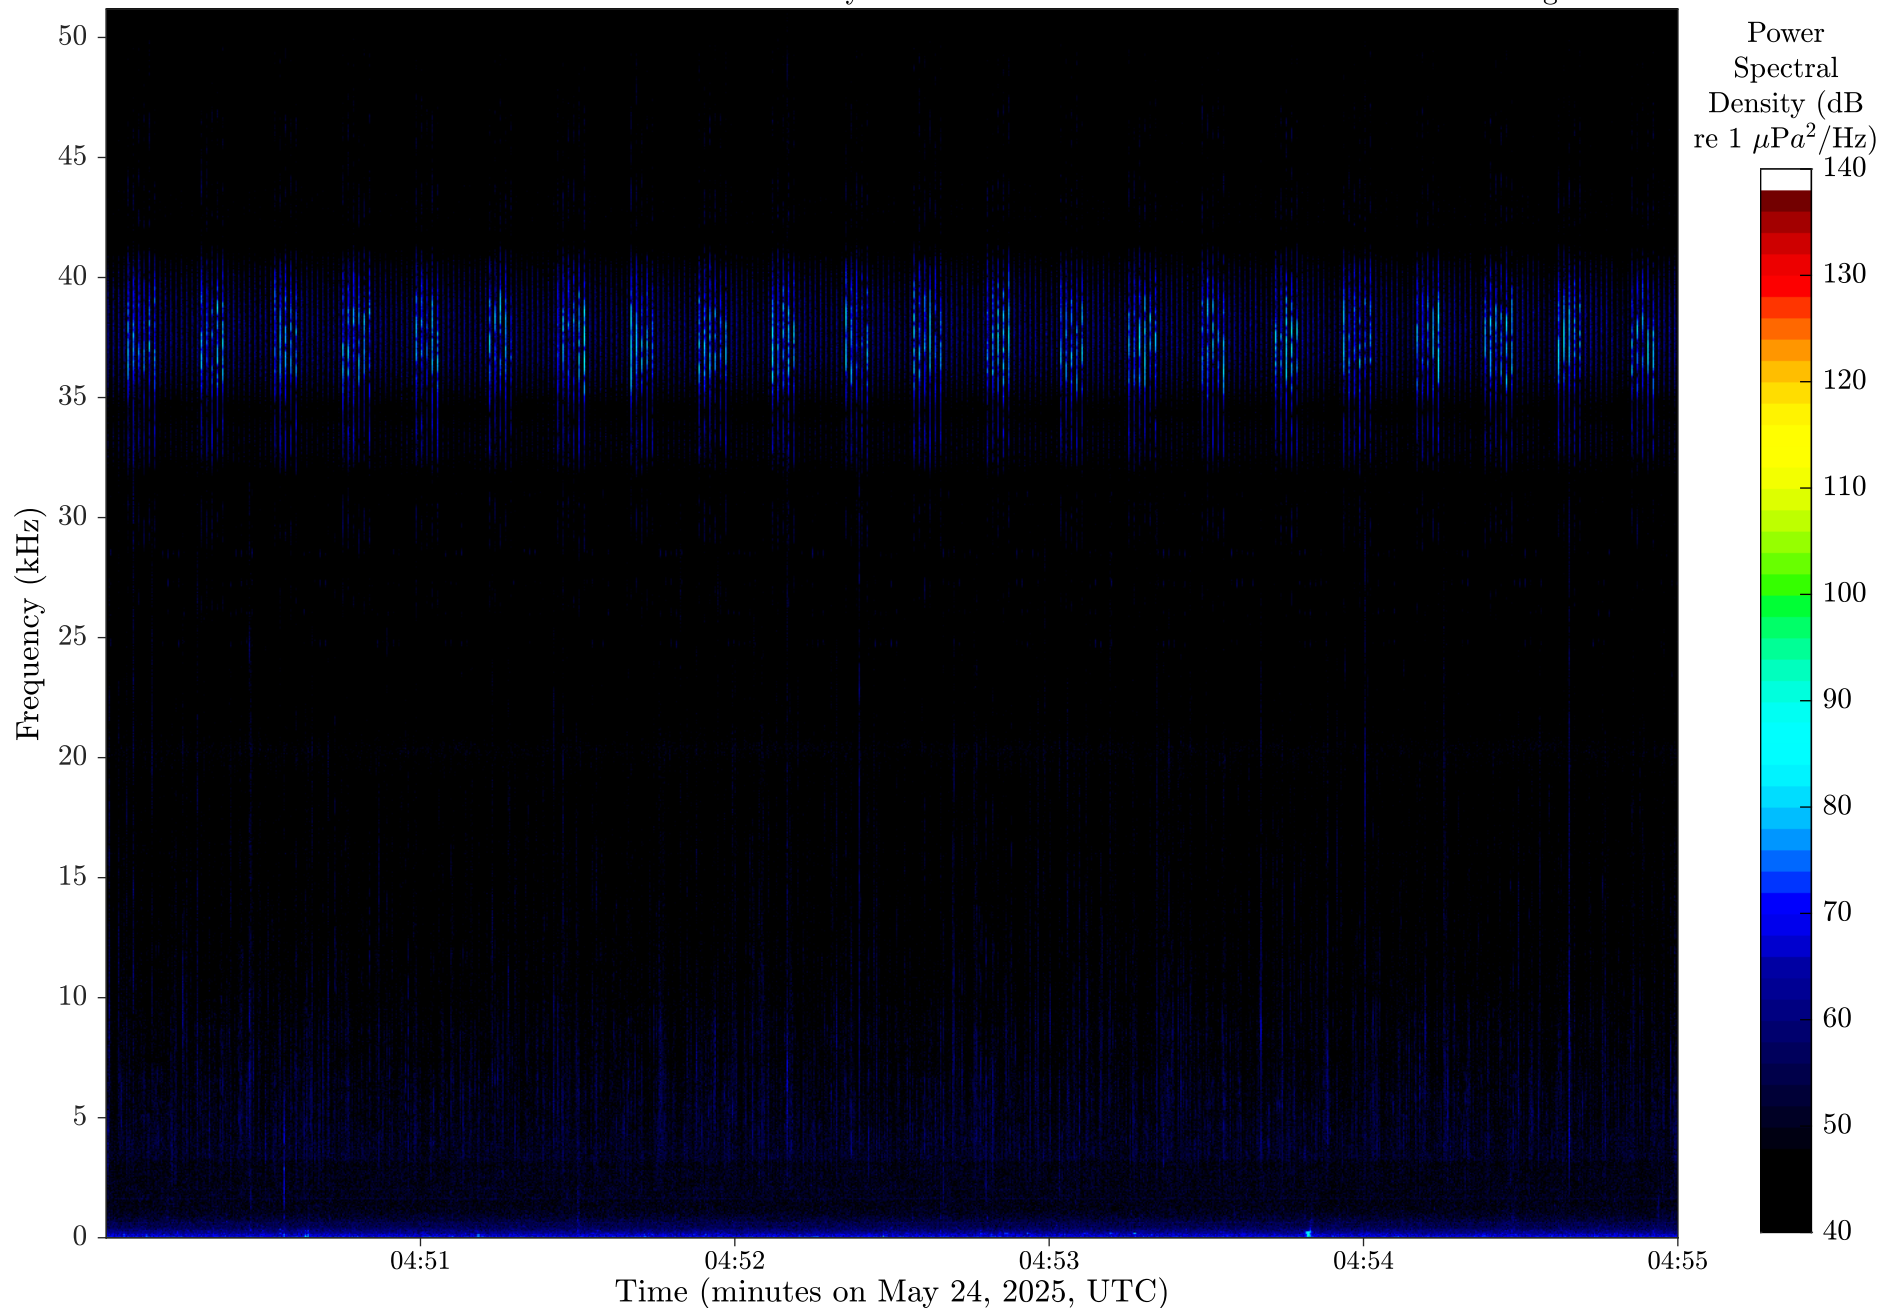


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:19:19 UTC

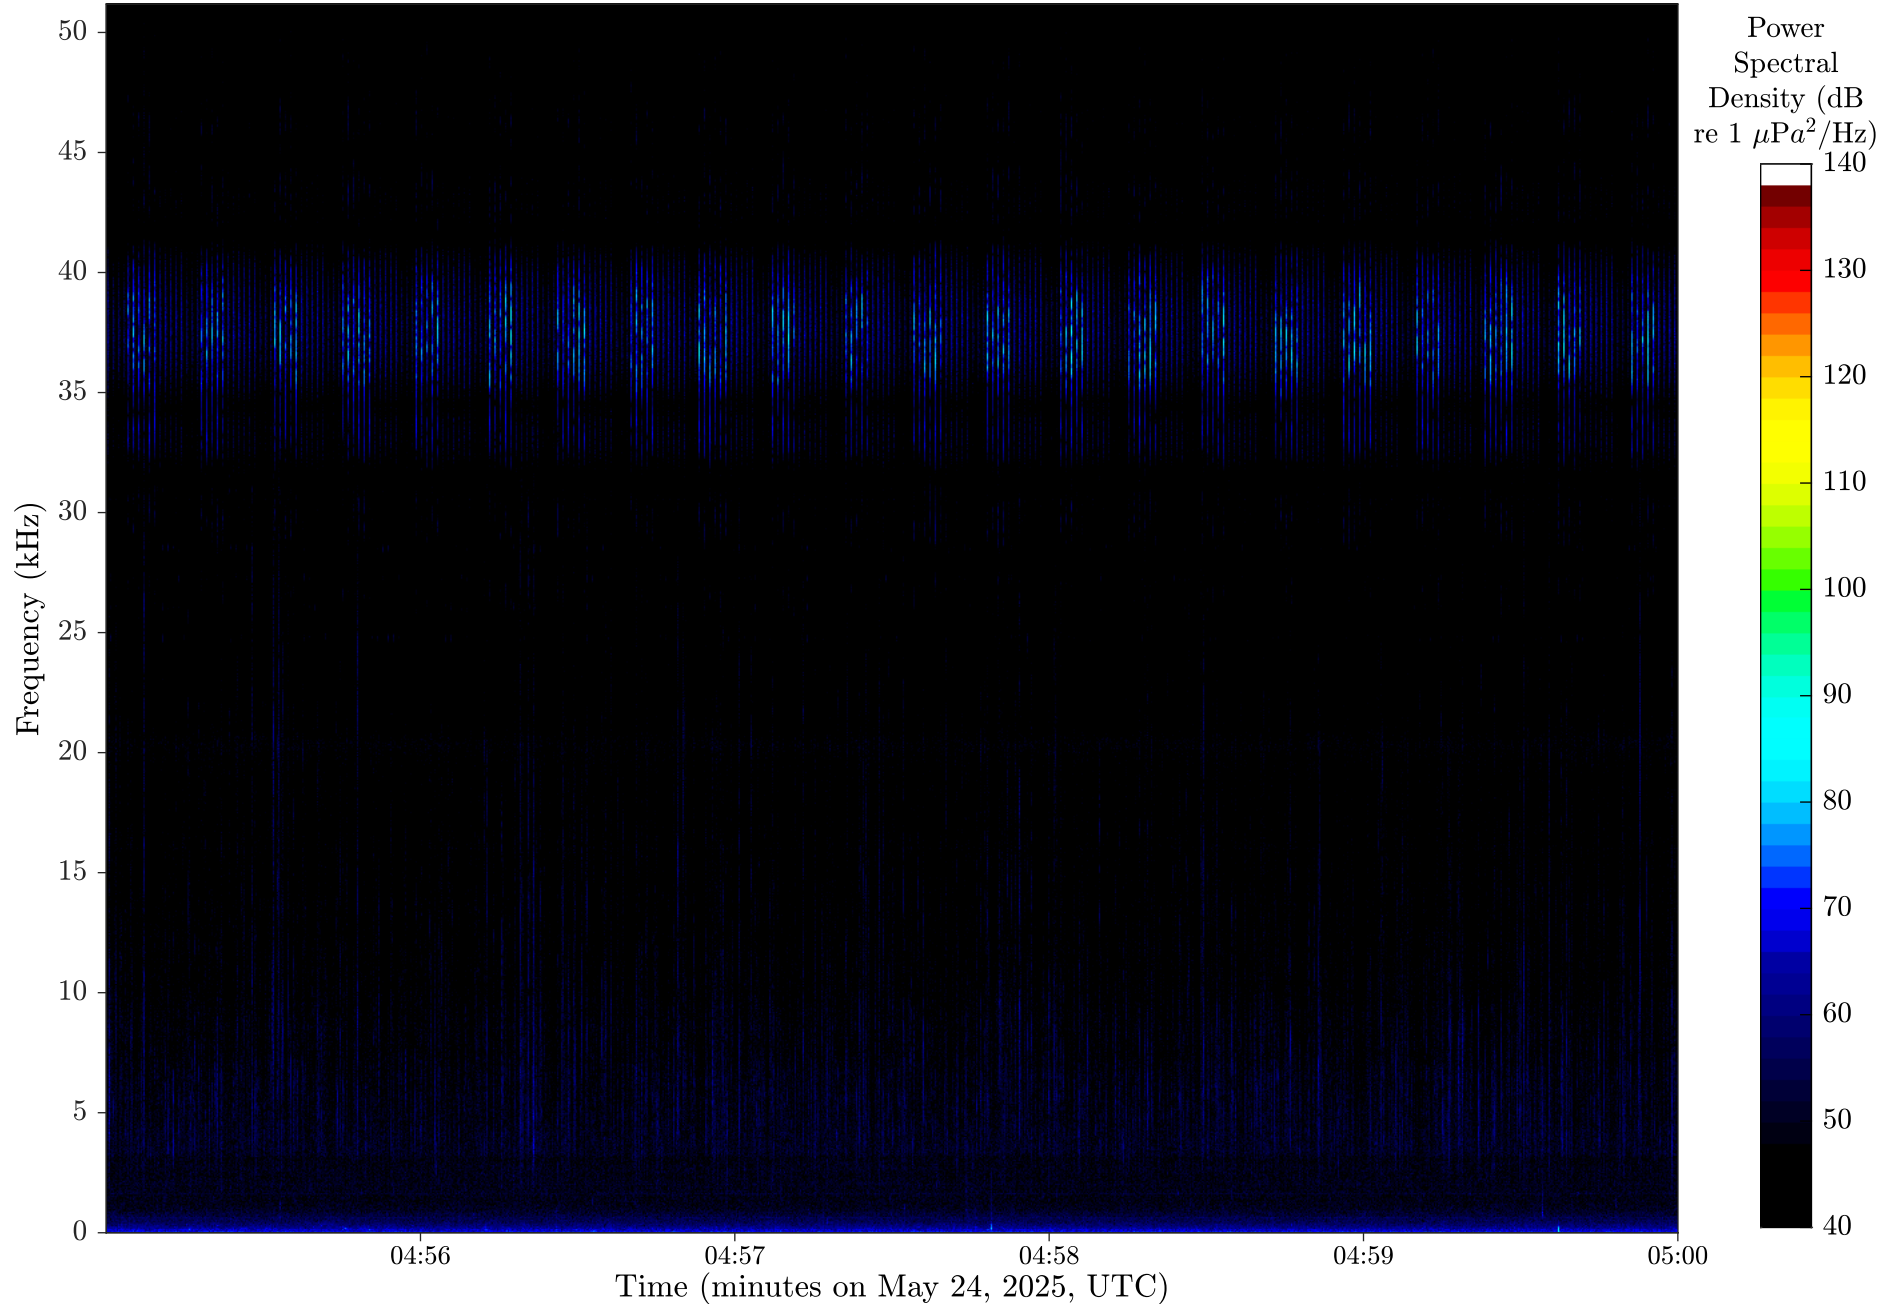


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:19:27 UTC

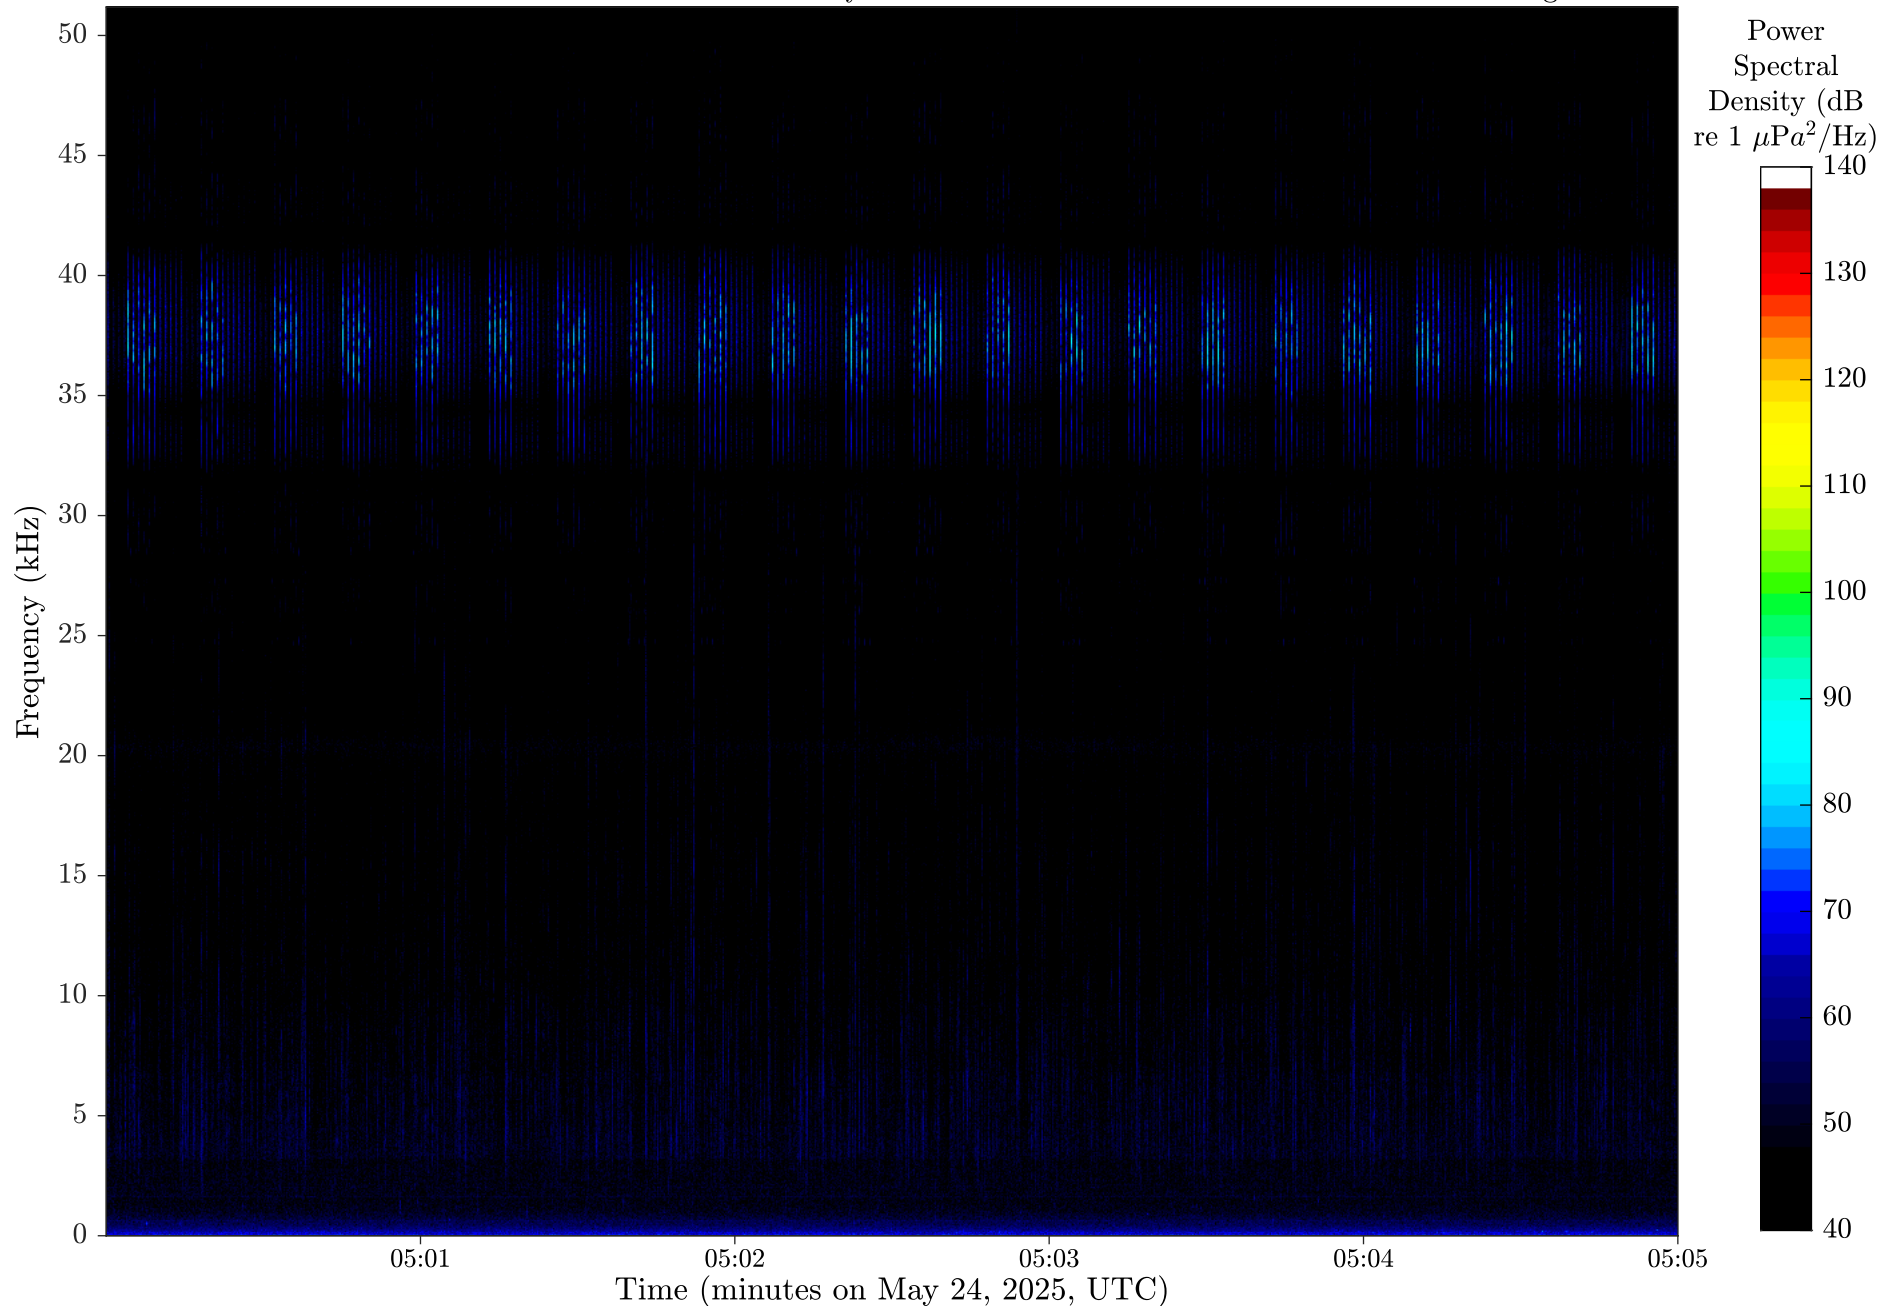


Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:19:34 UTC

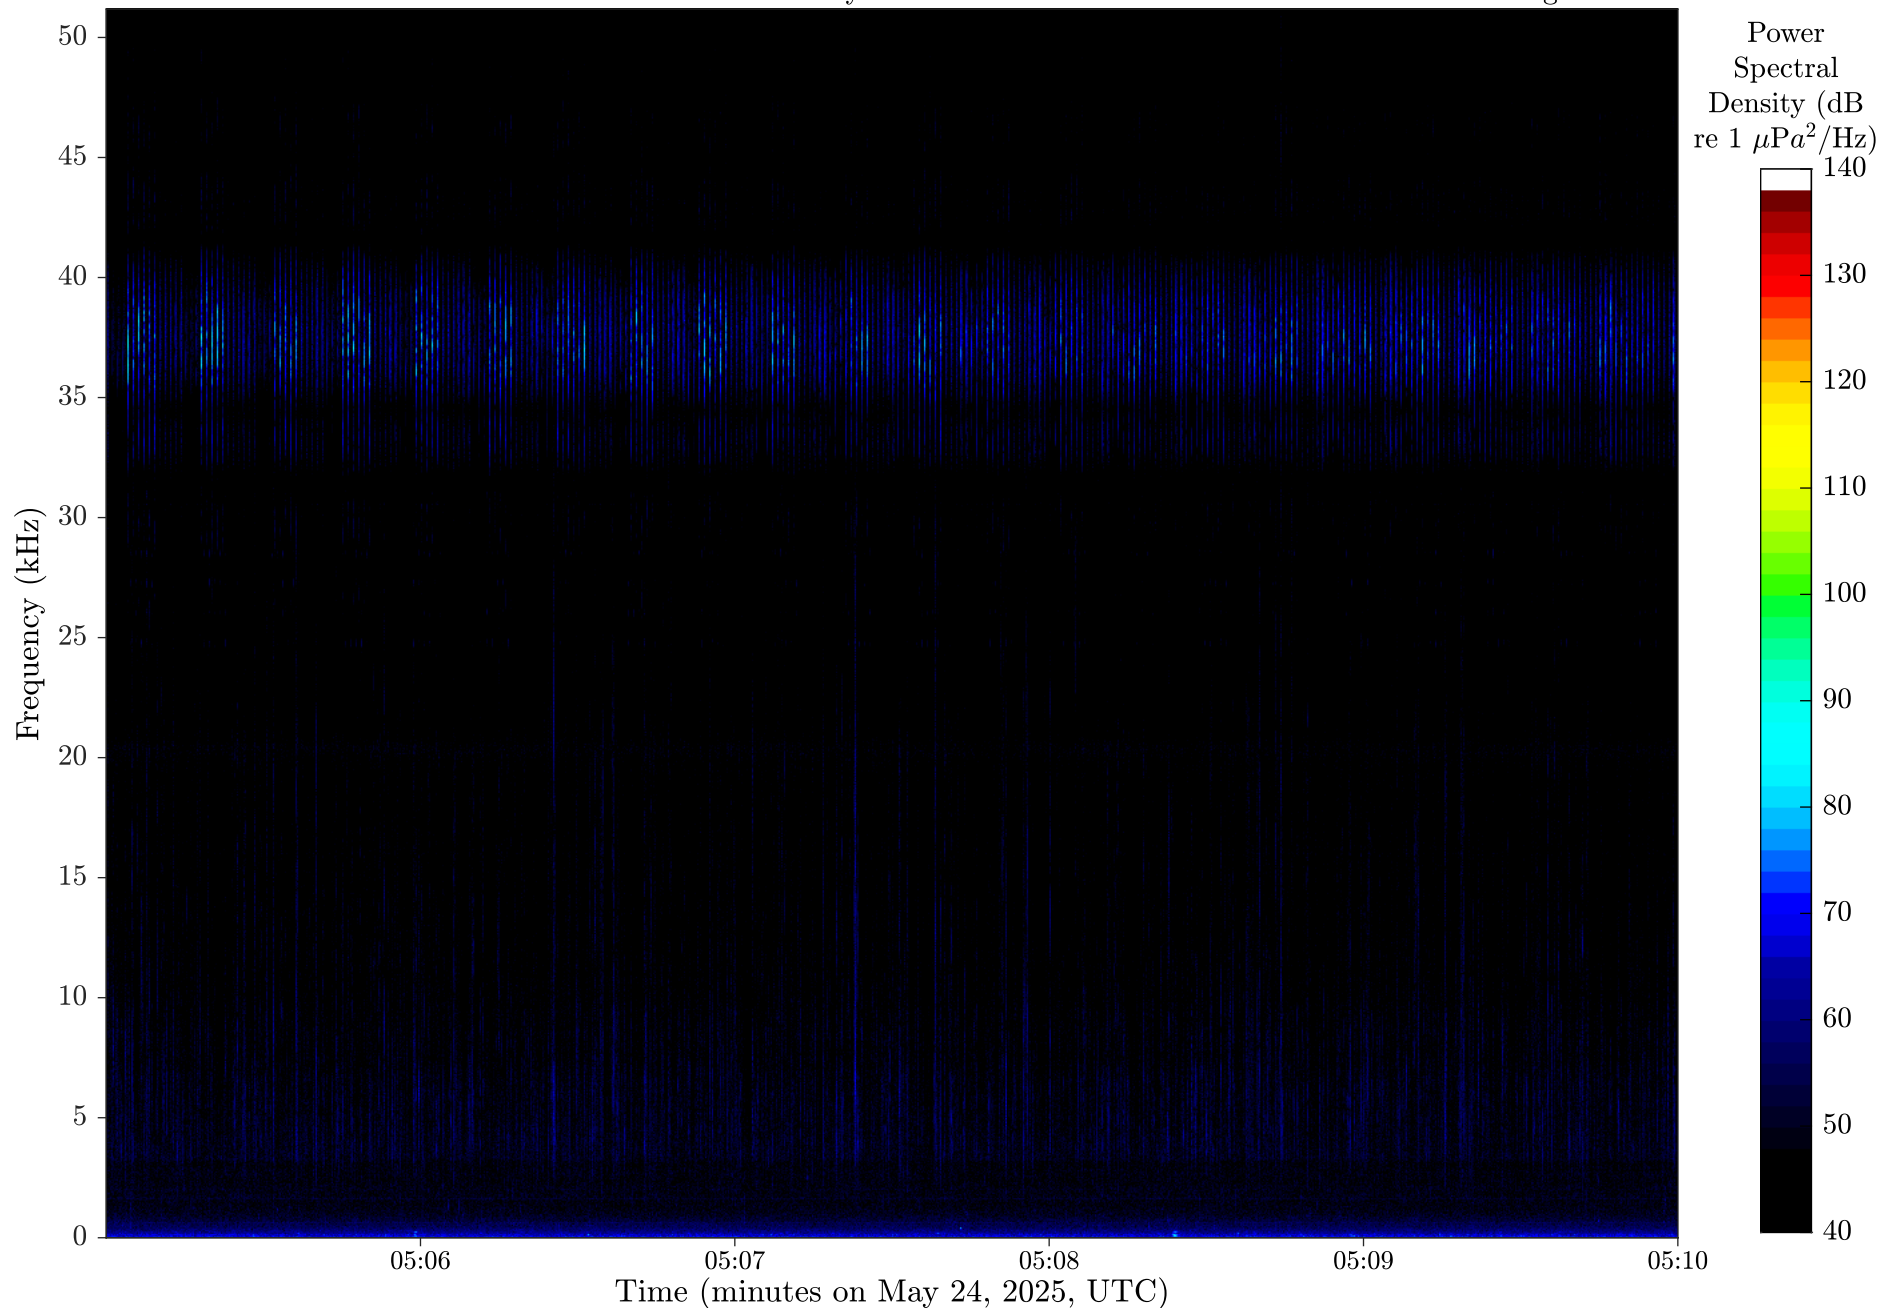


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:19:42 UTC

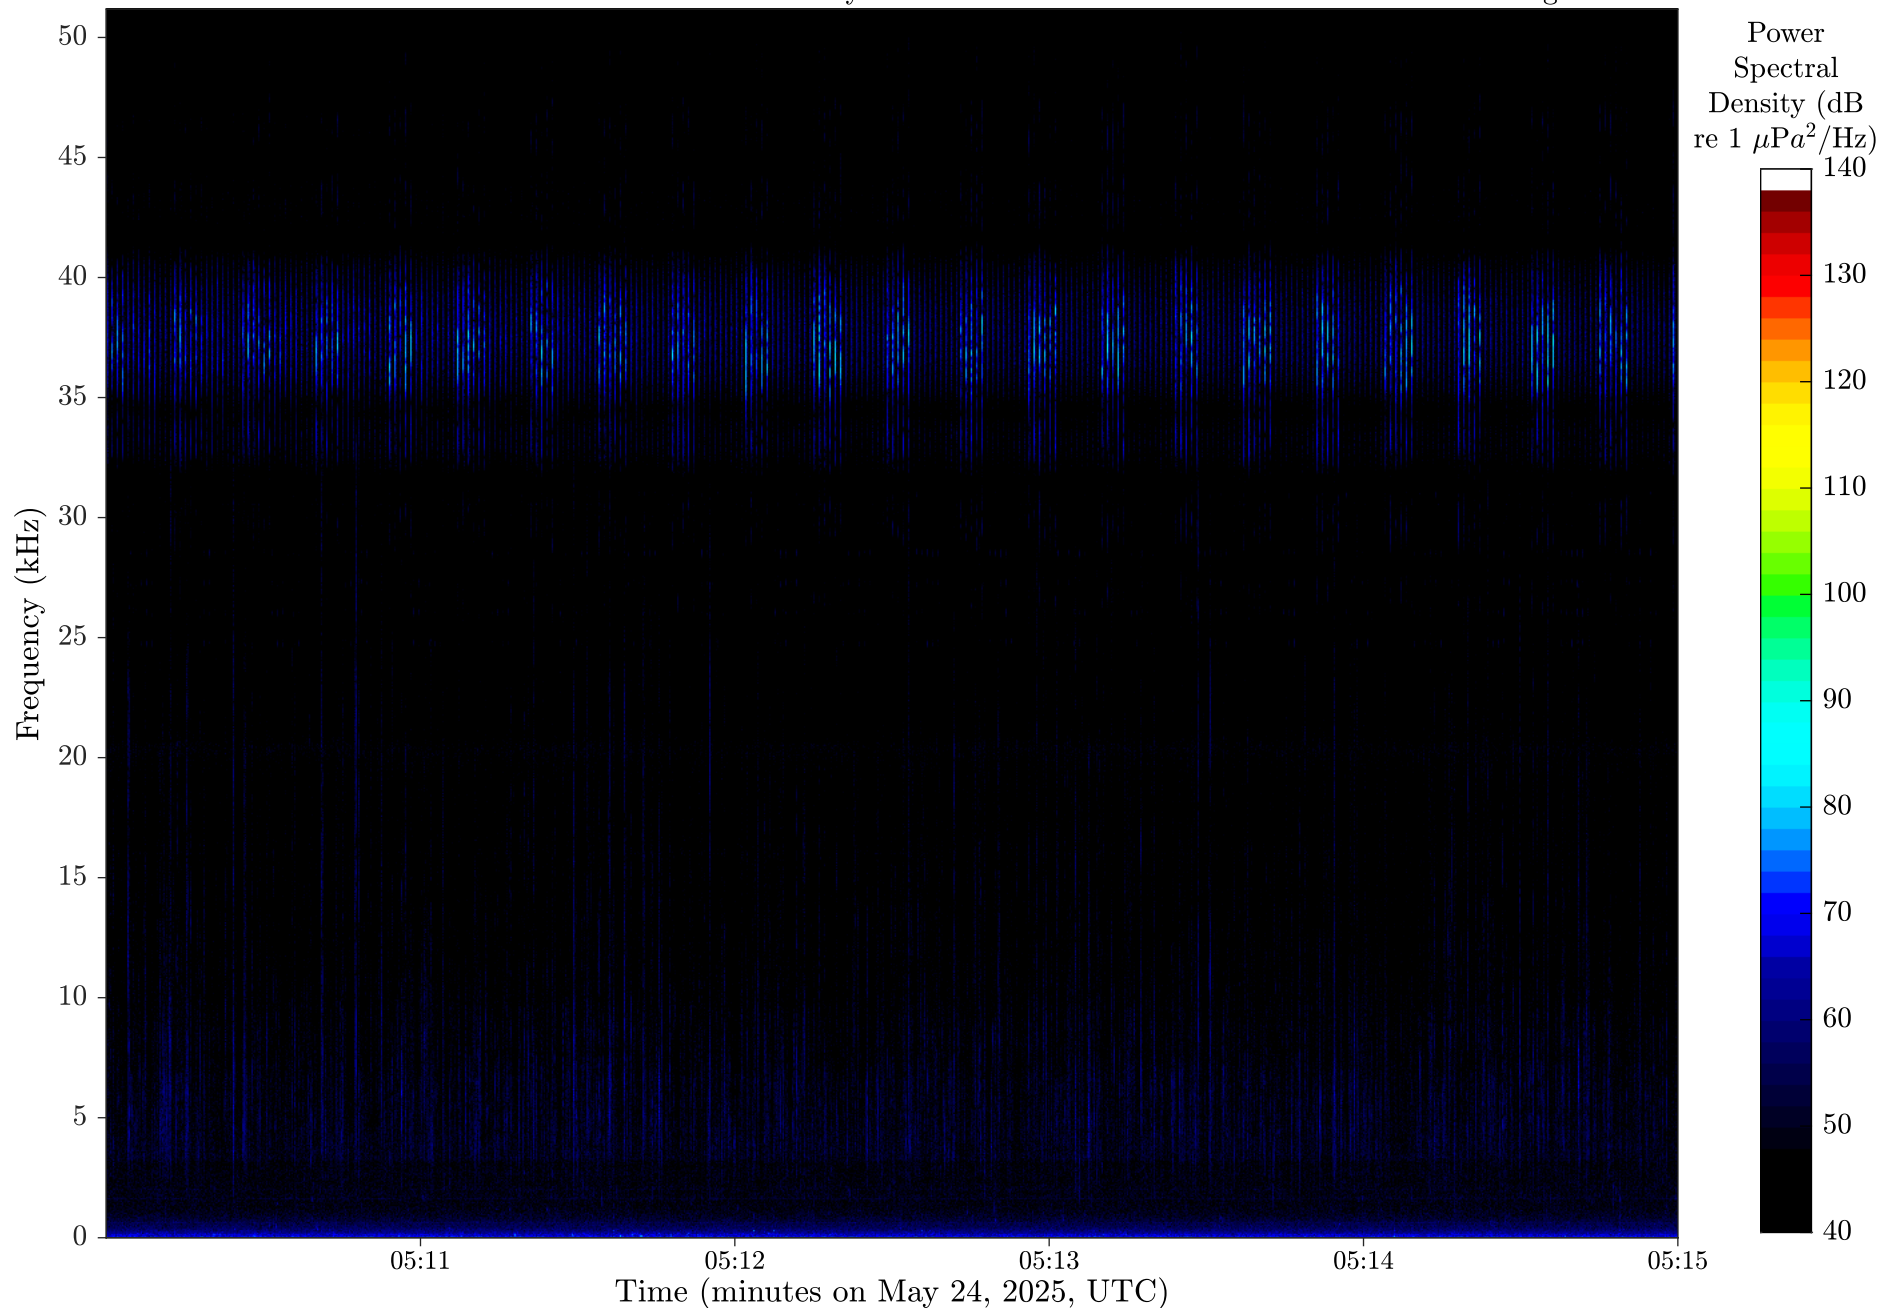

Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:19:49 UTC

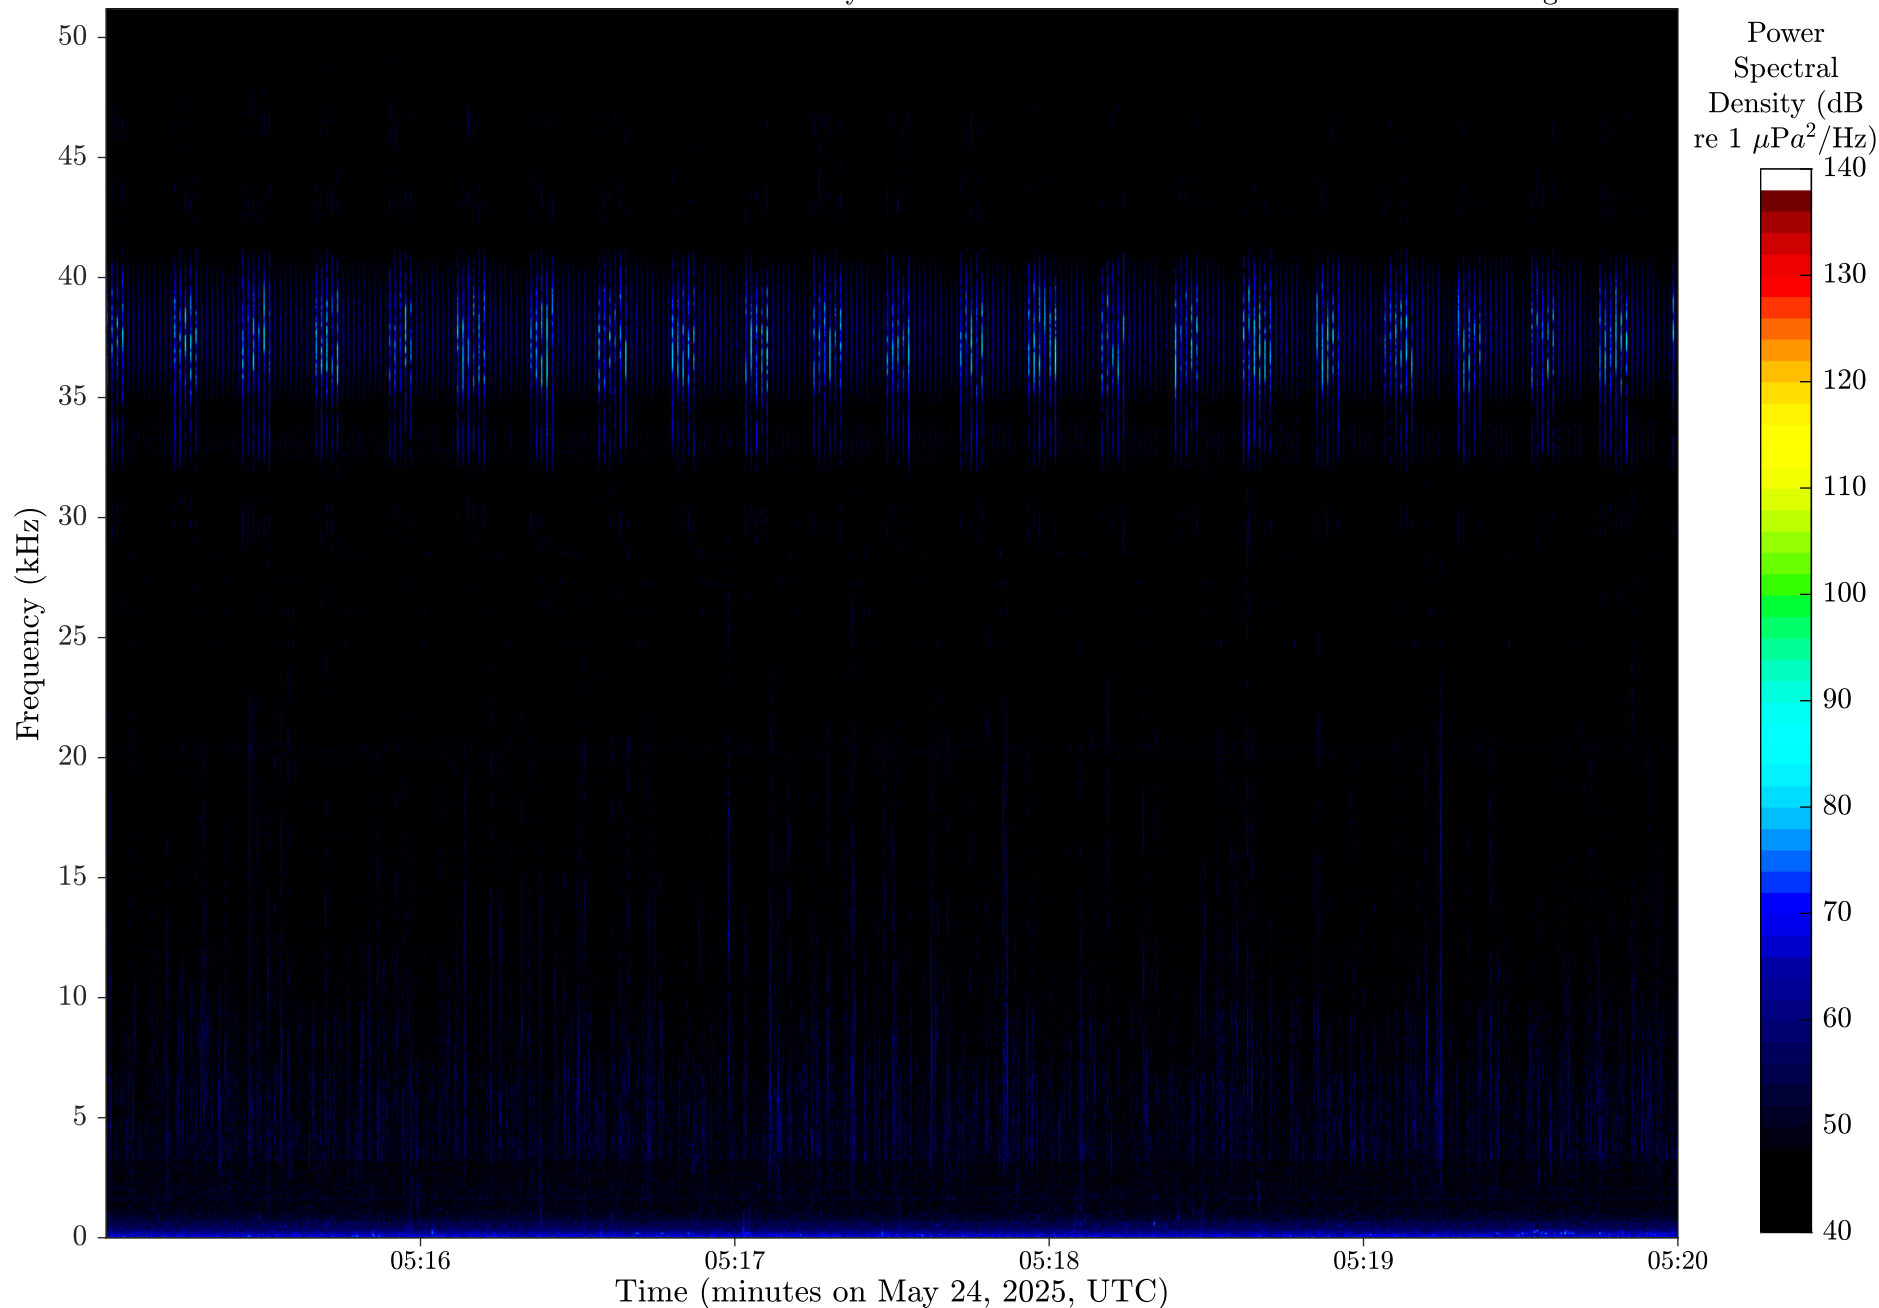

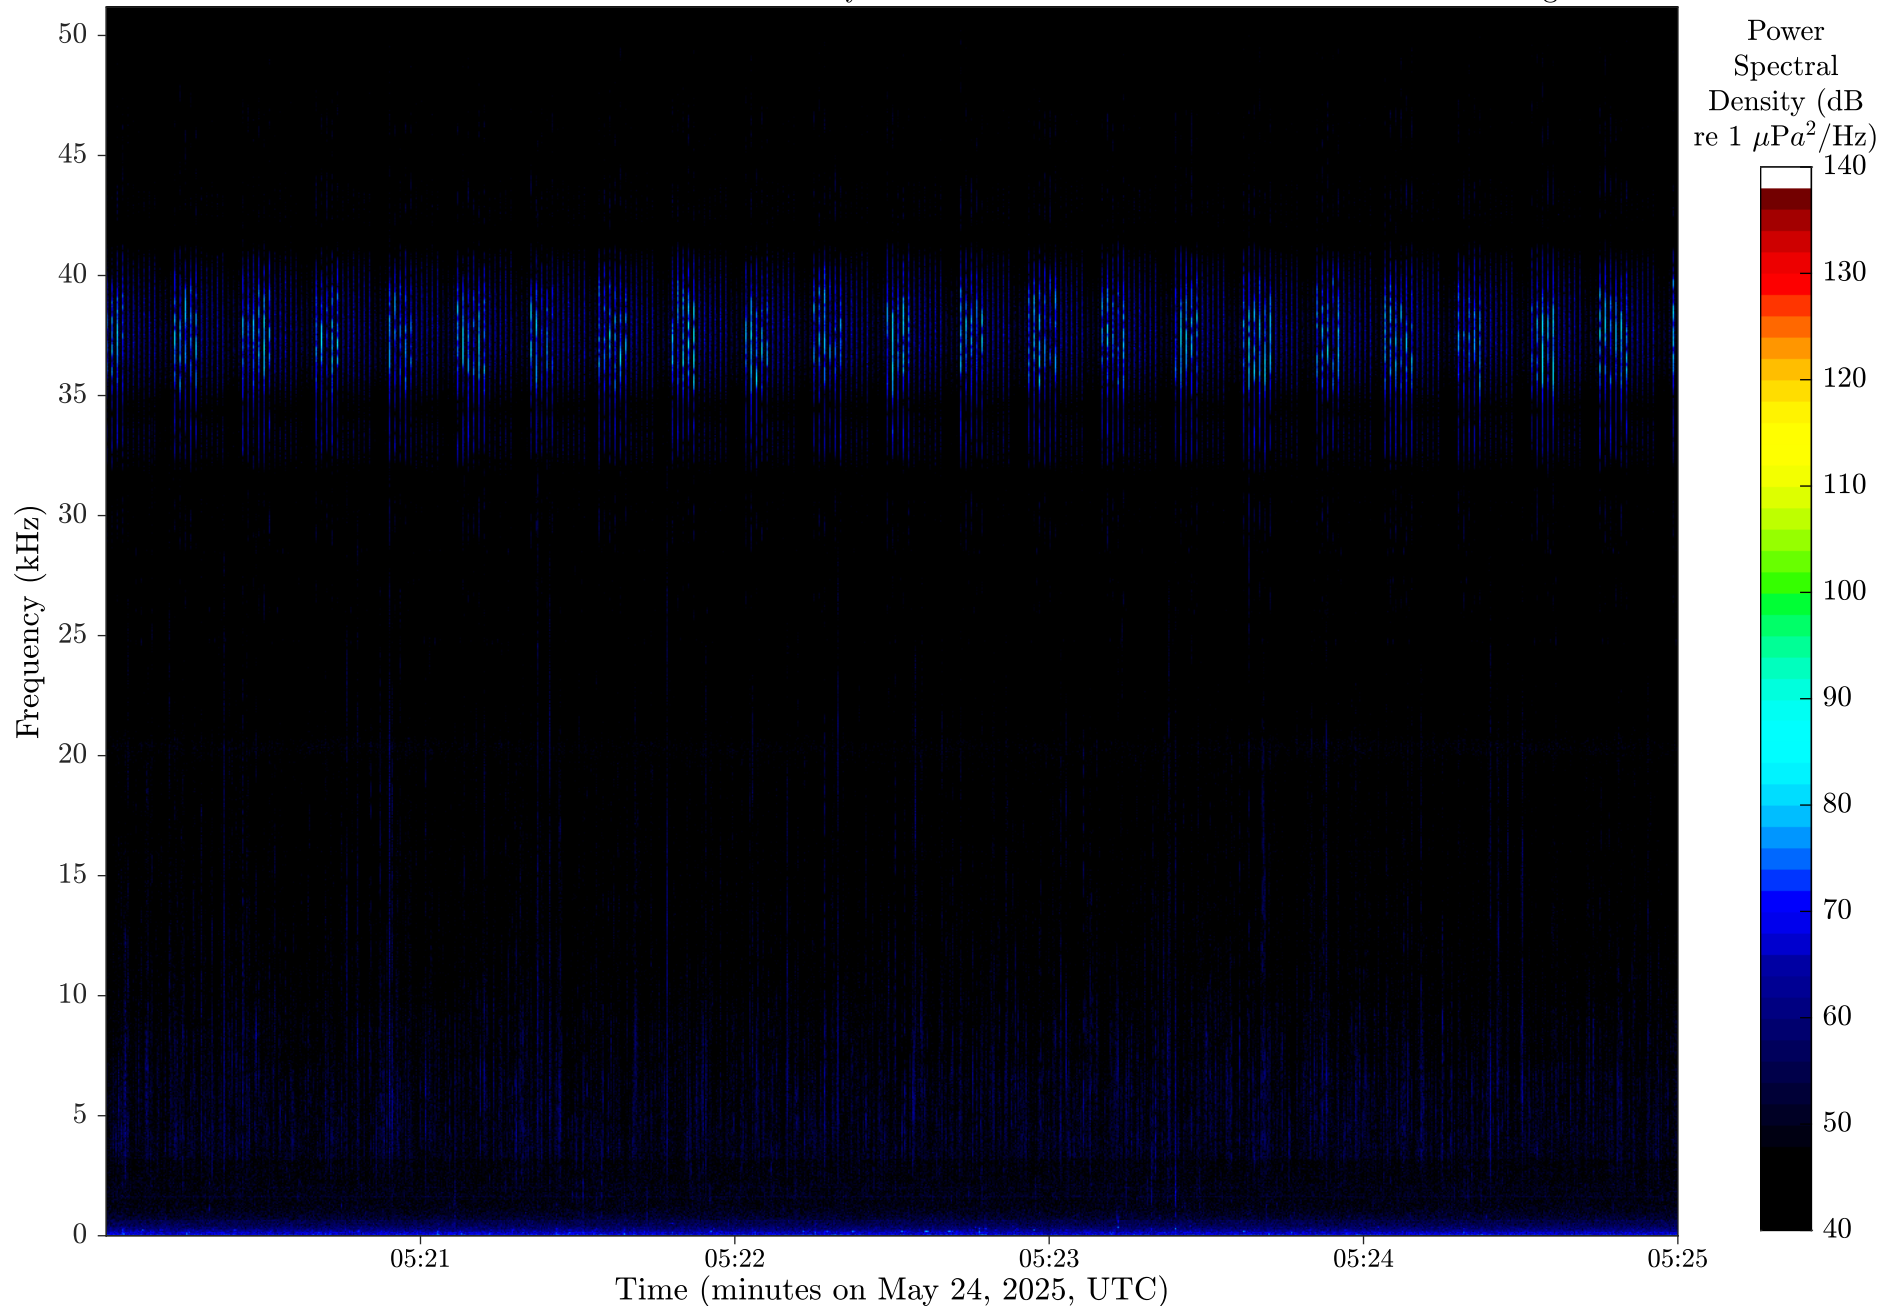


Comments: 36.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:03 UTC

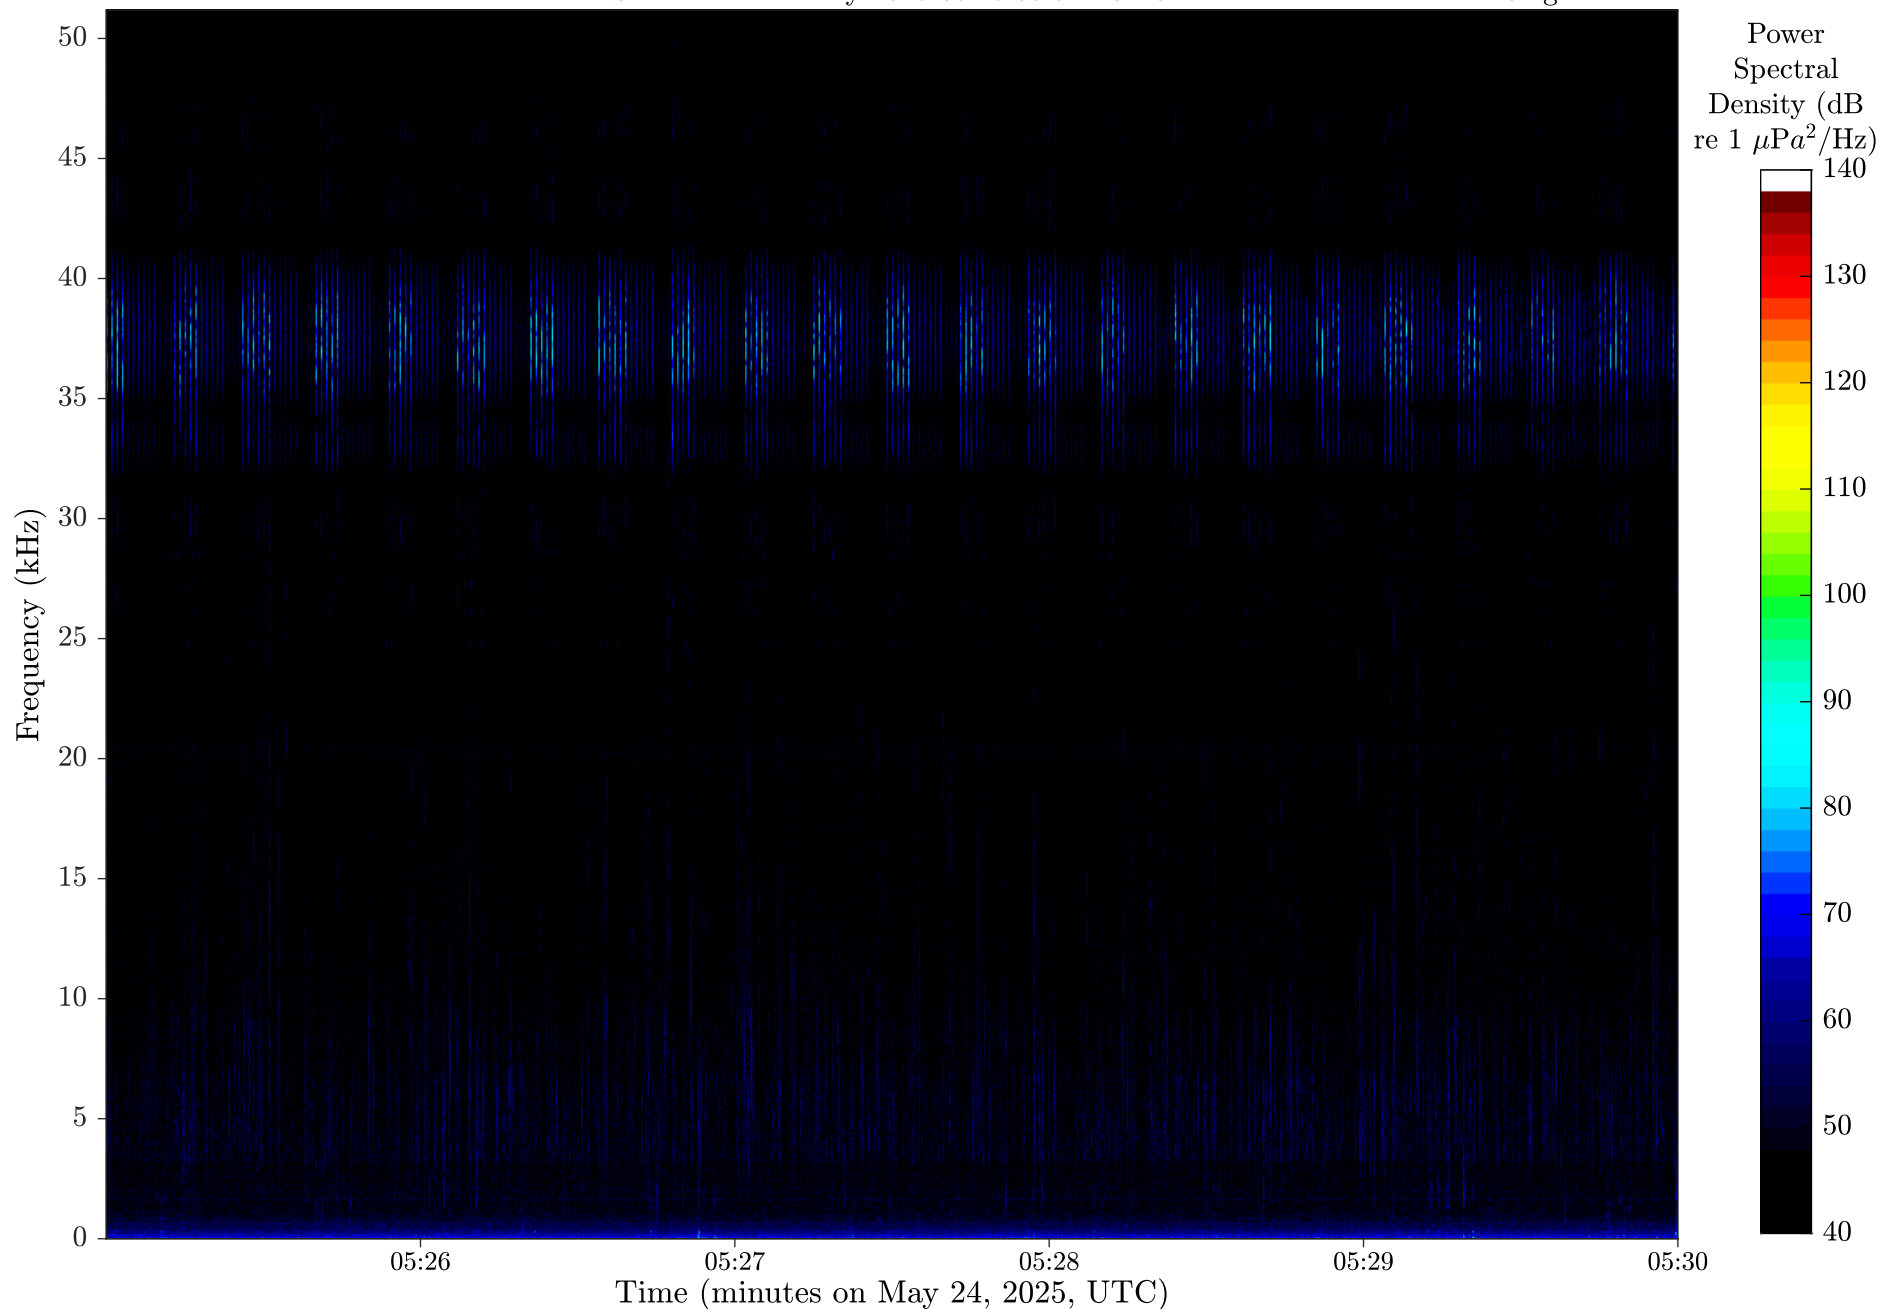


Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:10 UTC

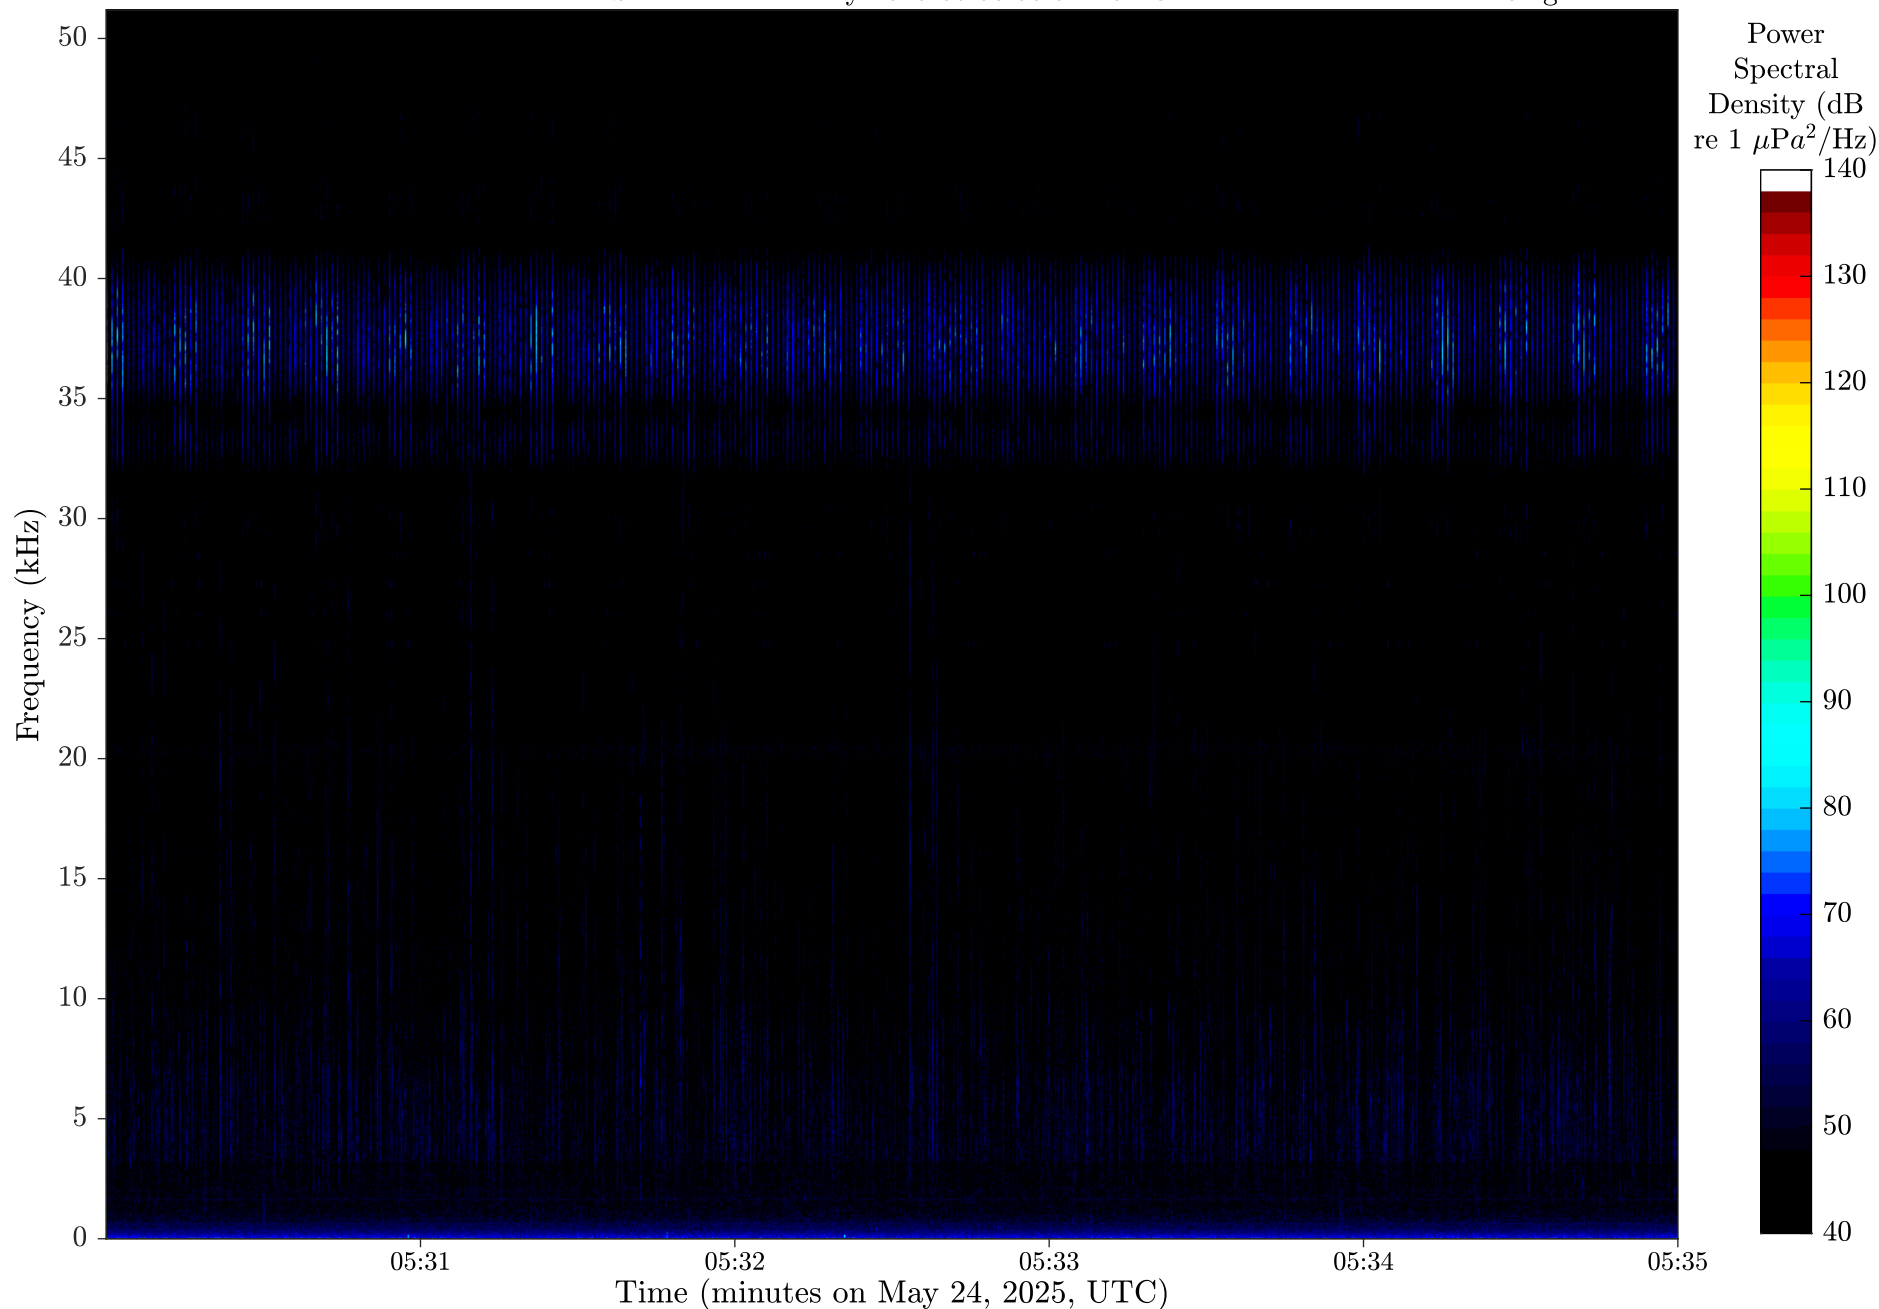


Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:17 UTC

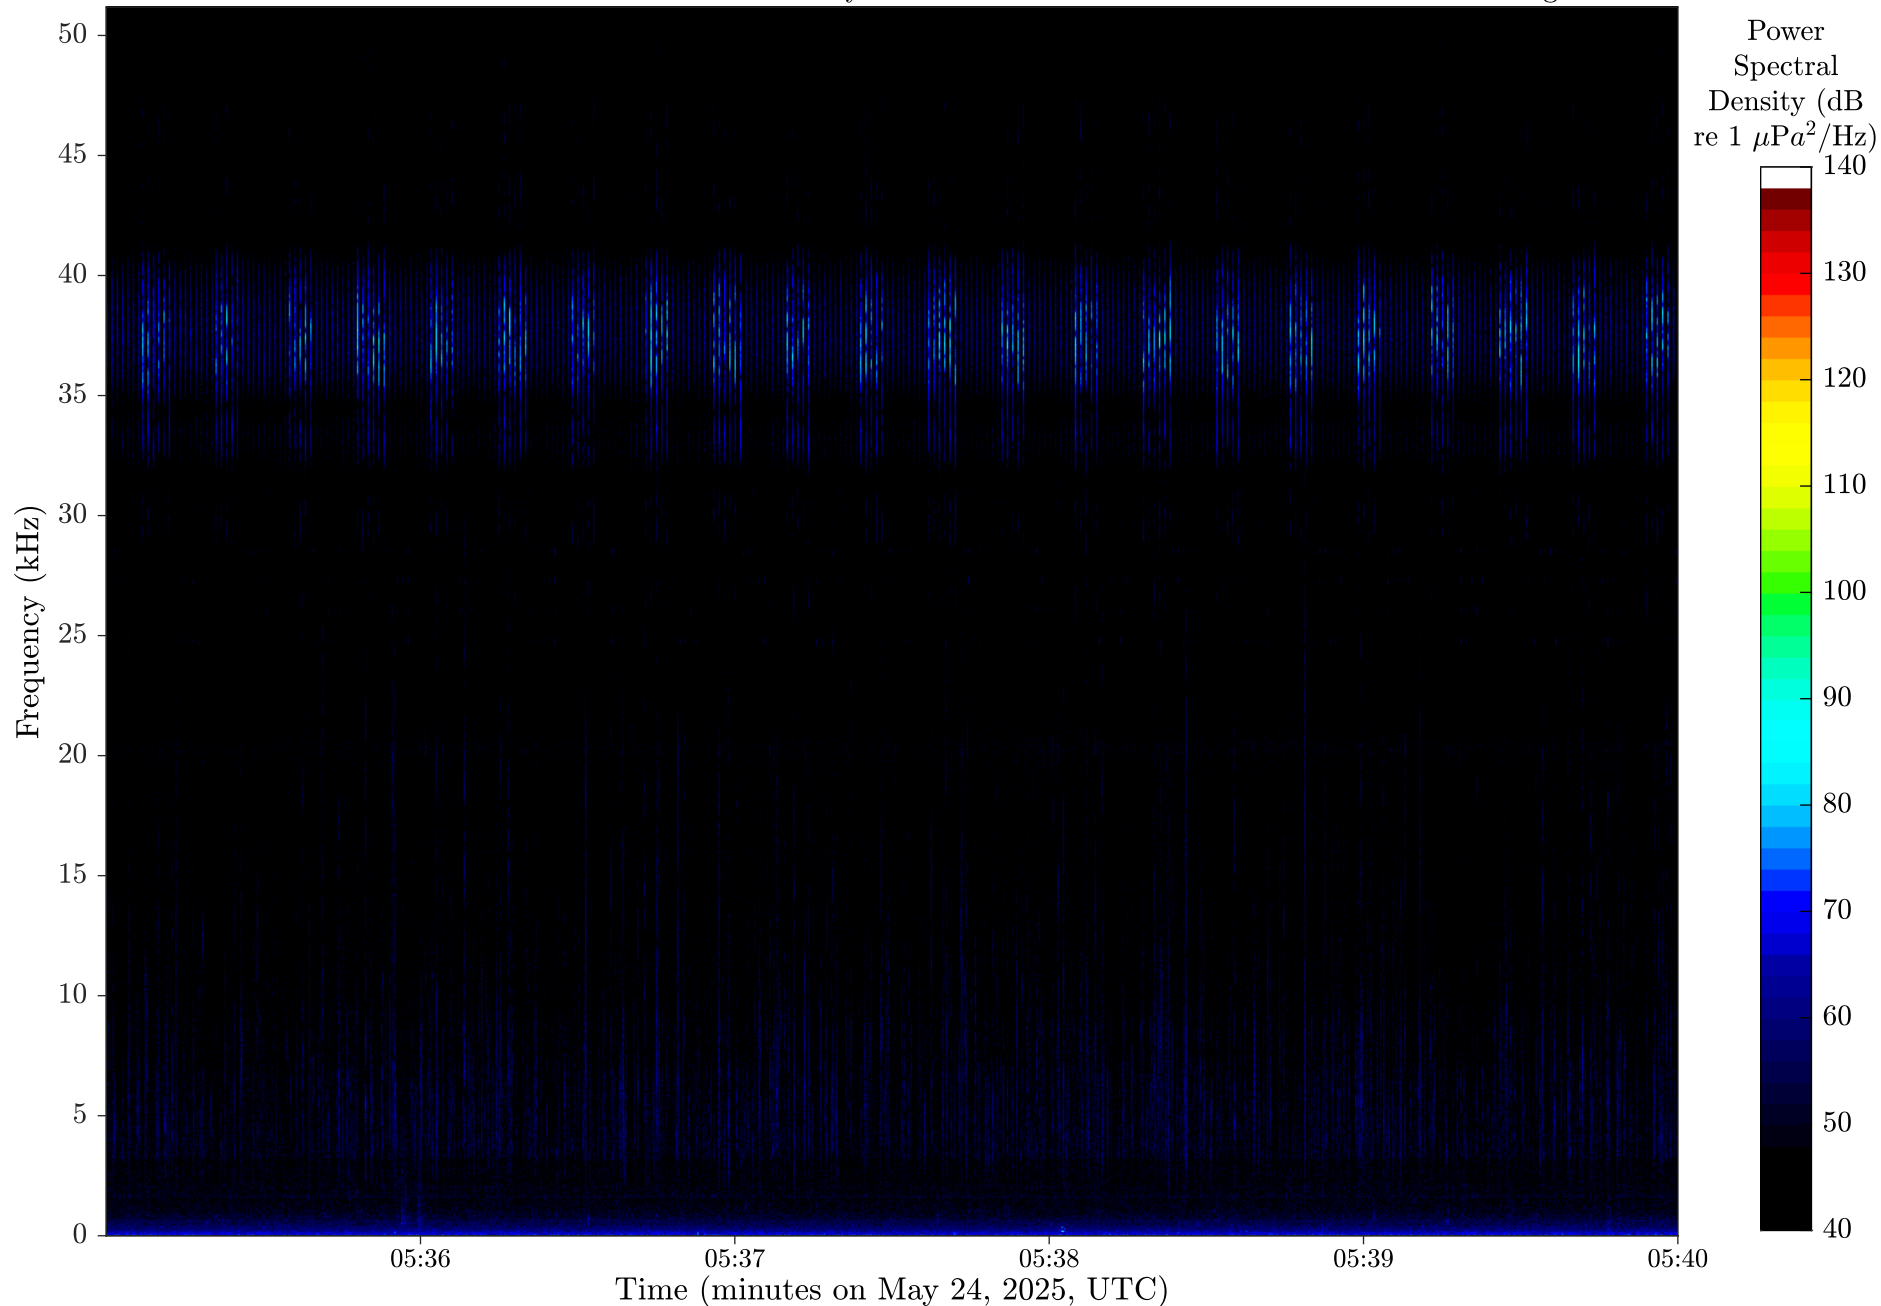


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:24 UTC

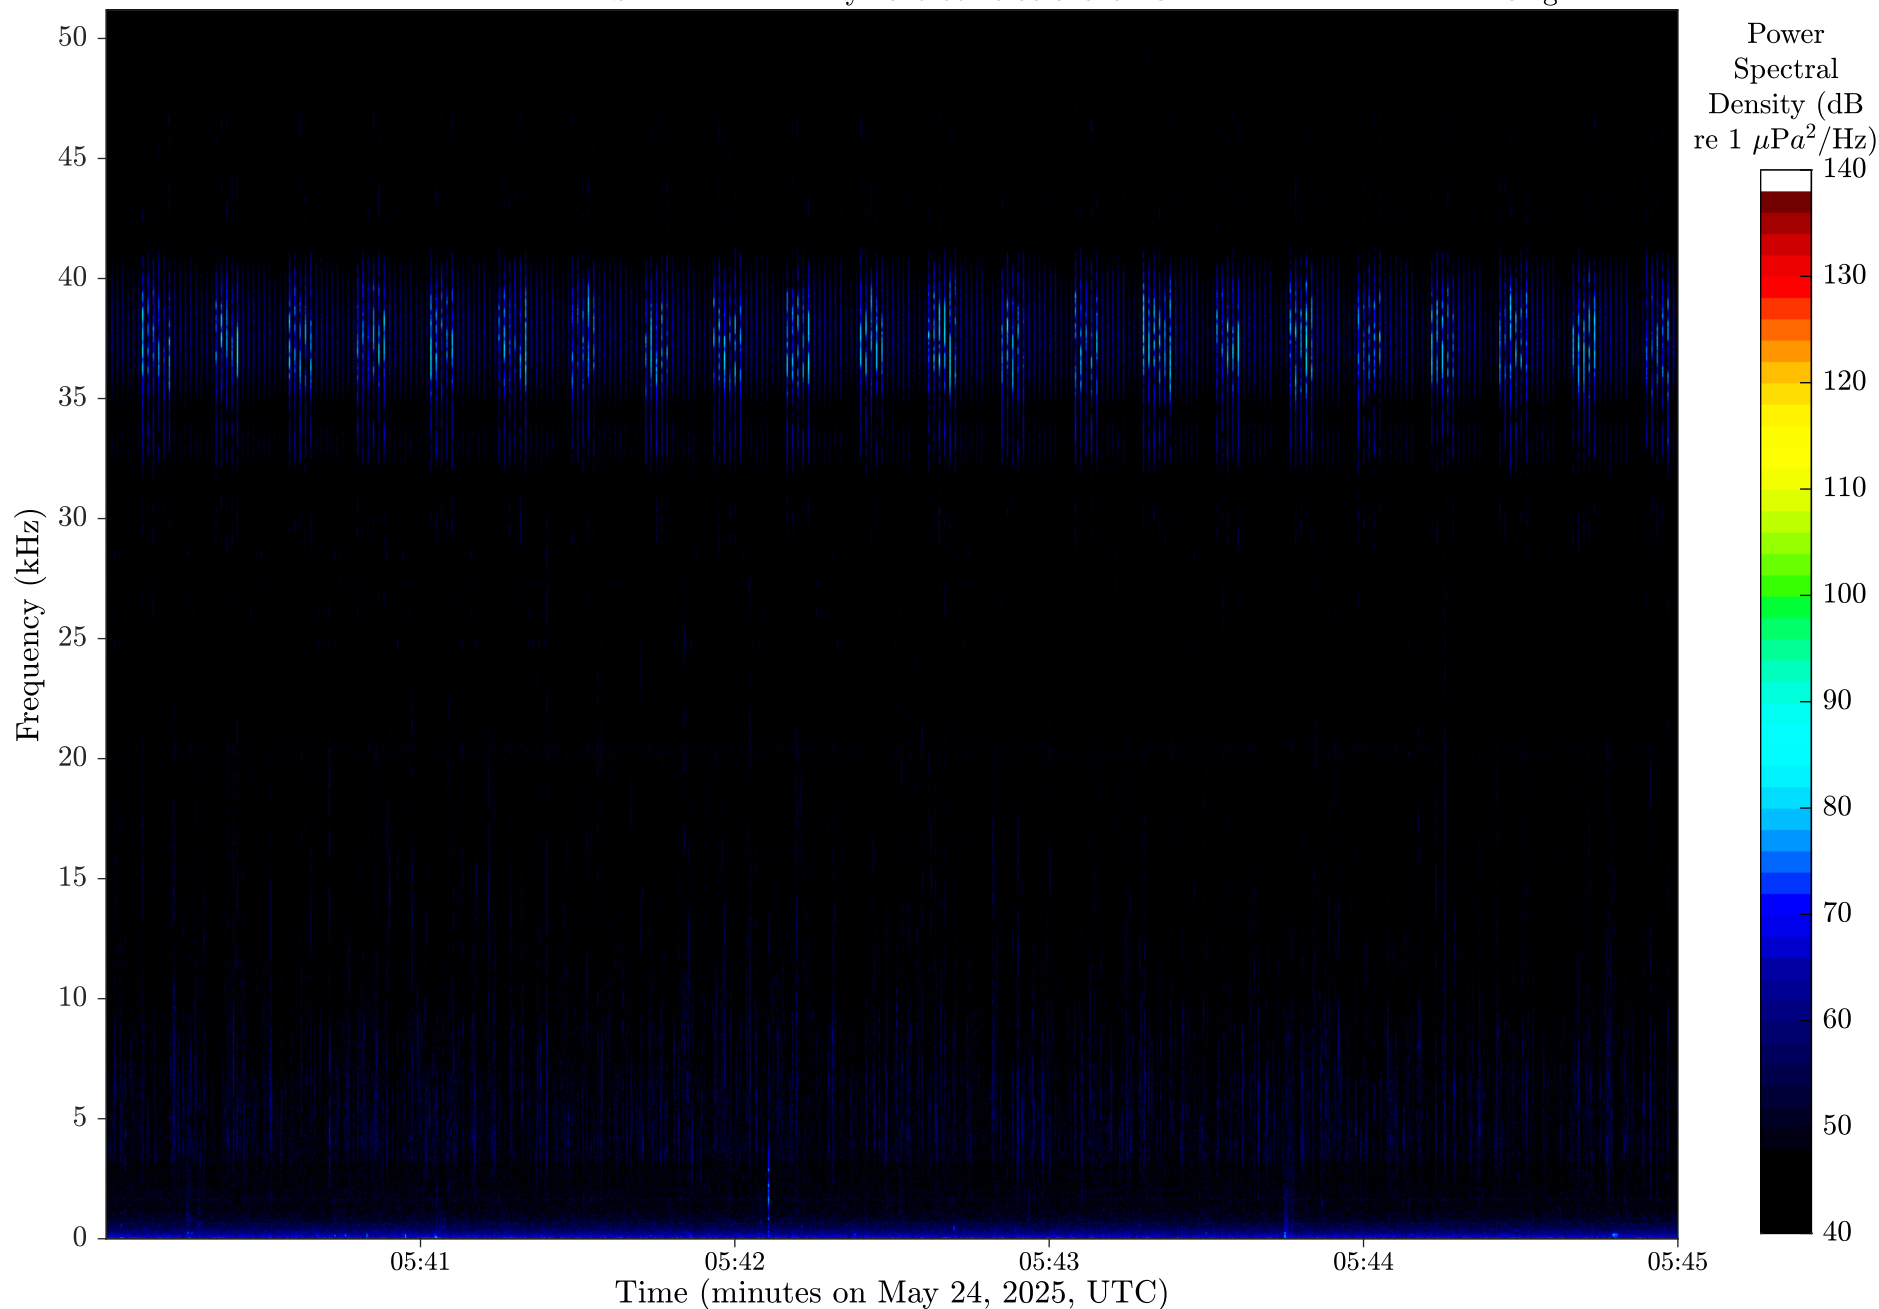


Comments: 36.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:31 UTC

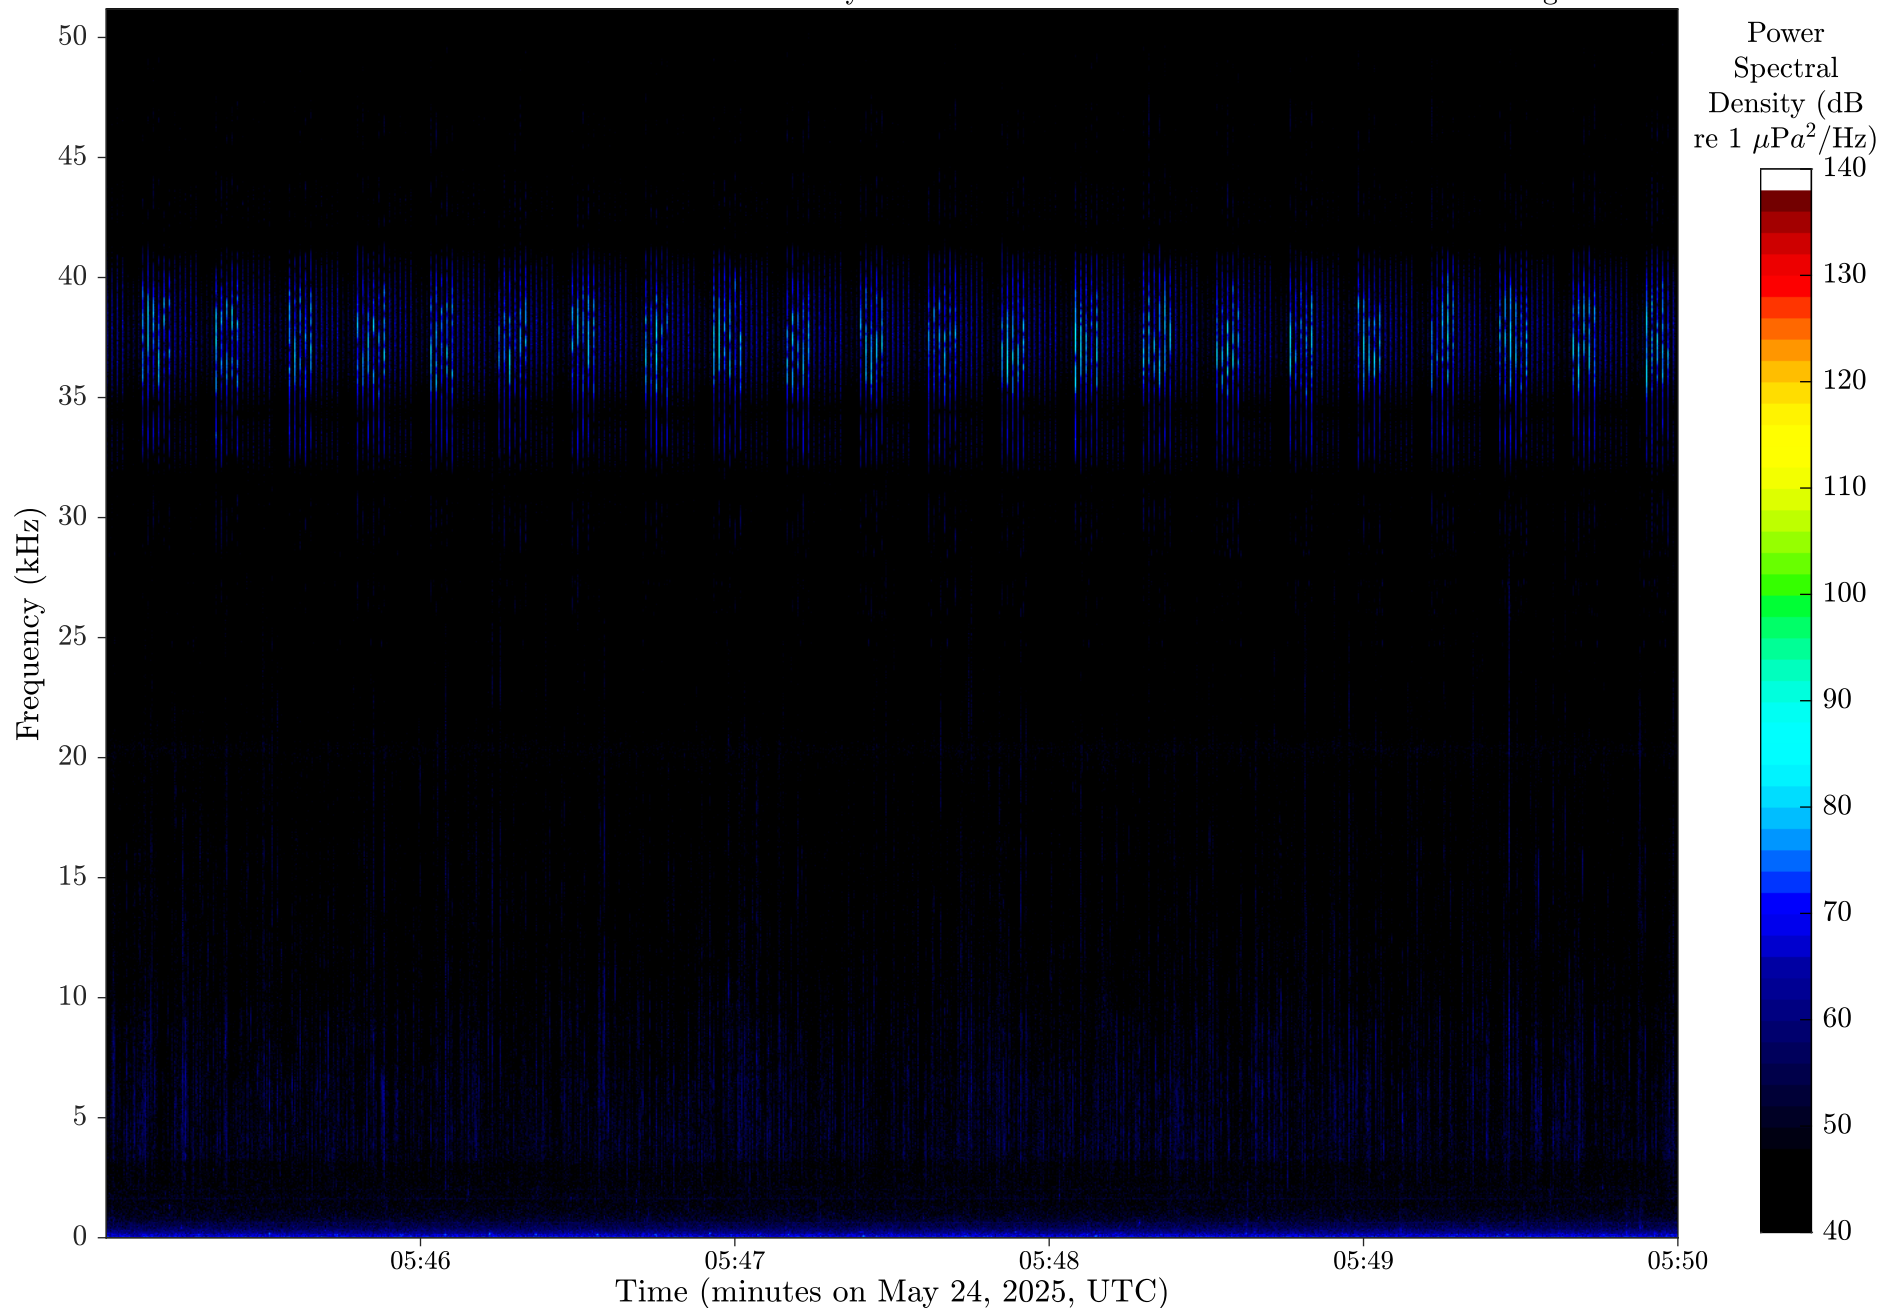


Comments: 36.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:20:38 UTC

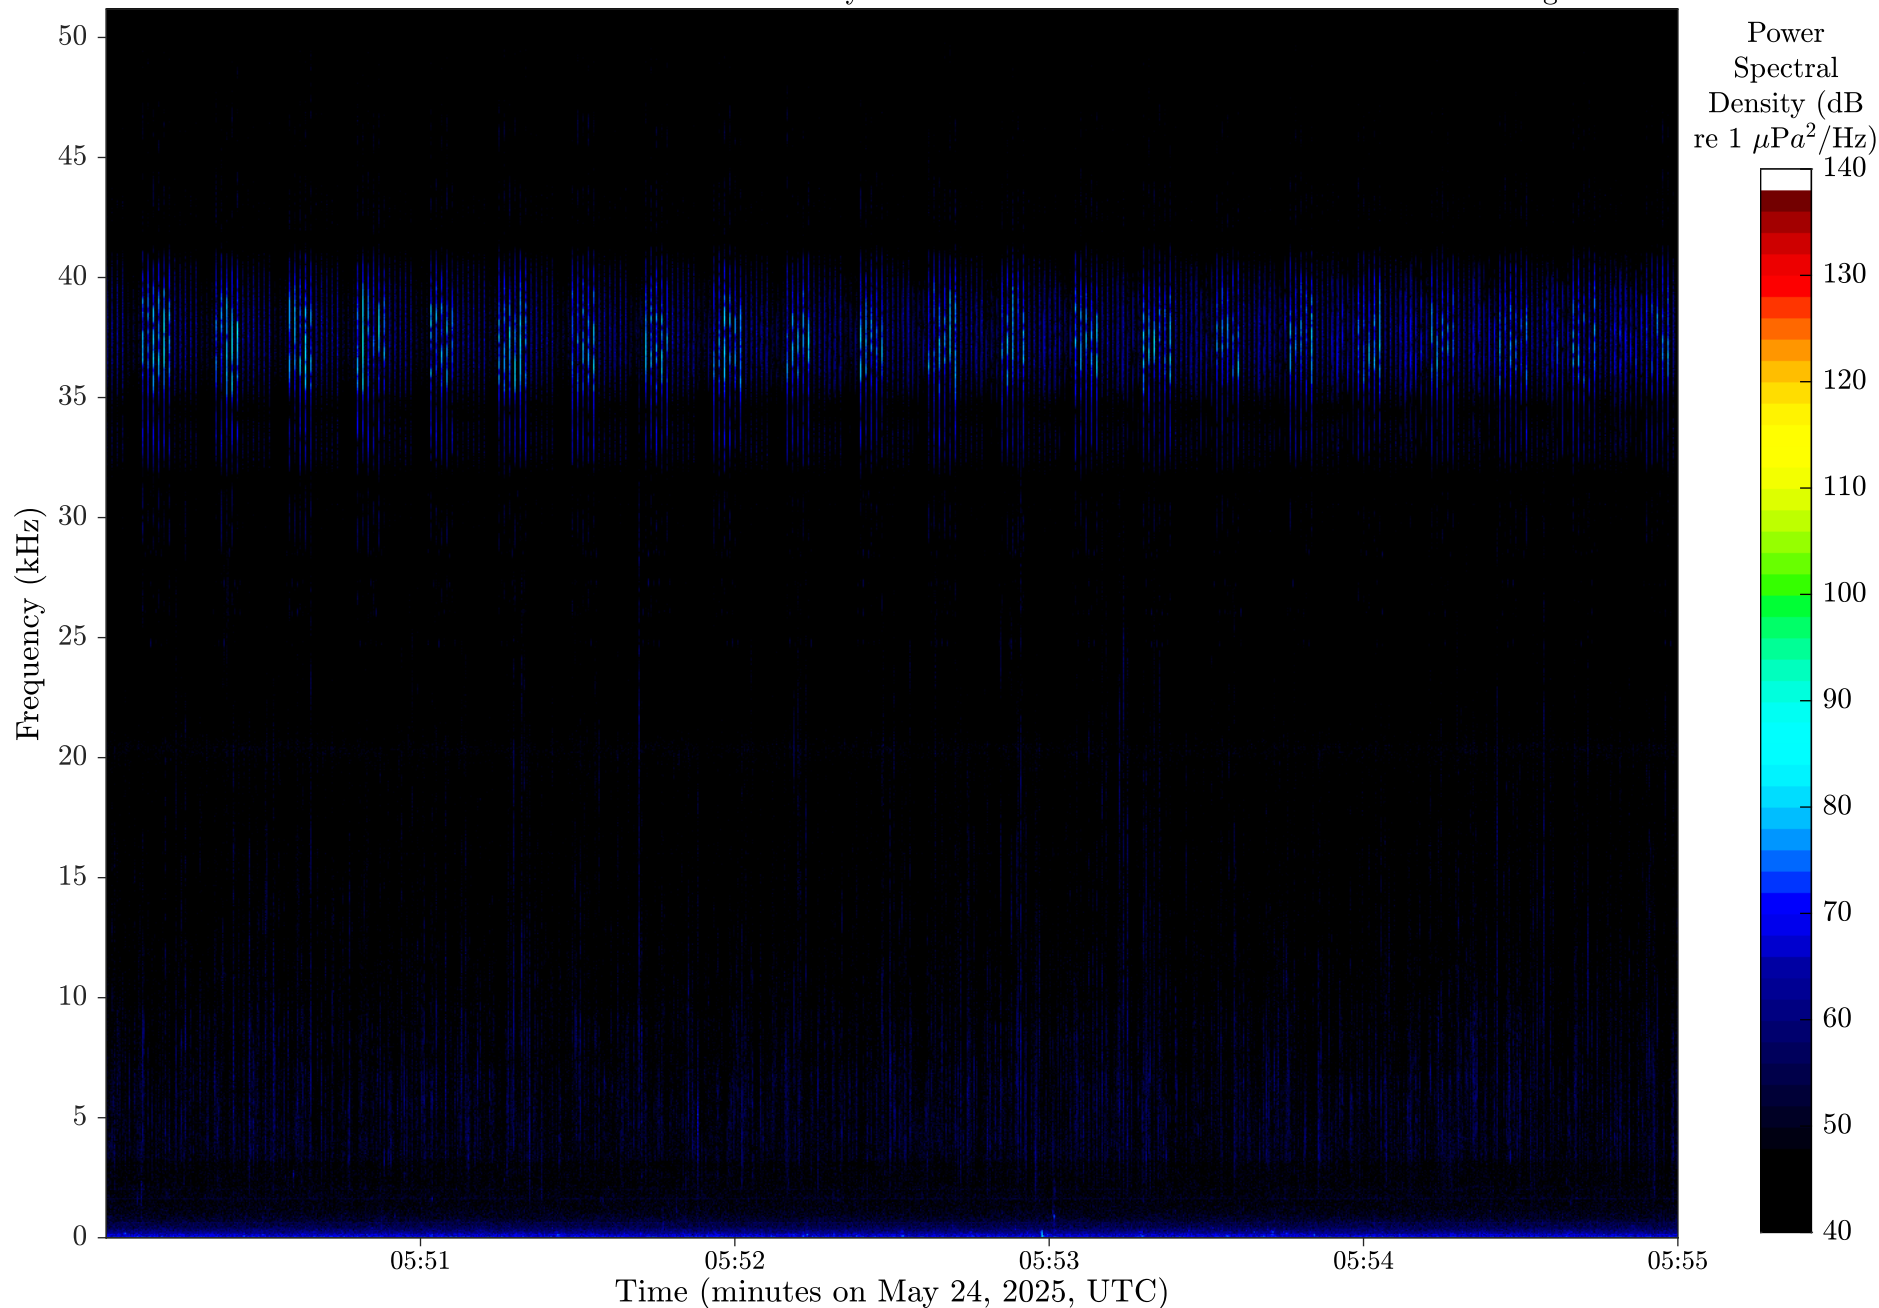

Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:20:46 UTC

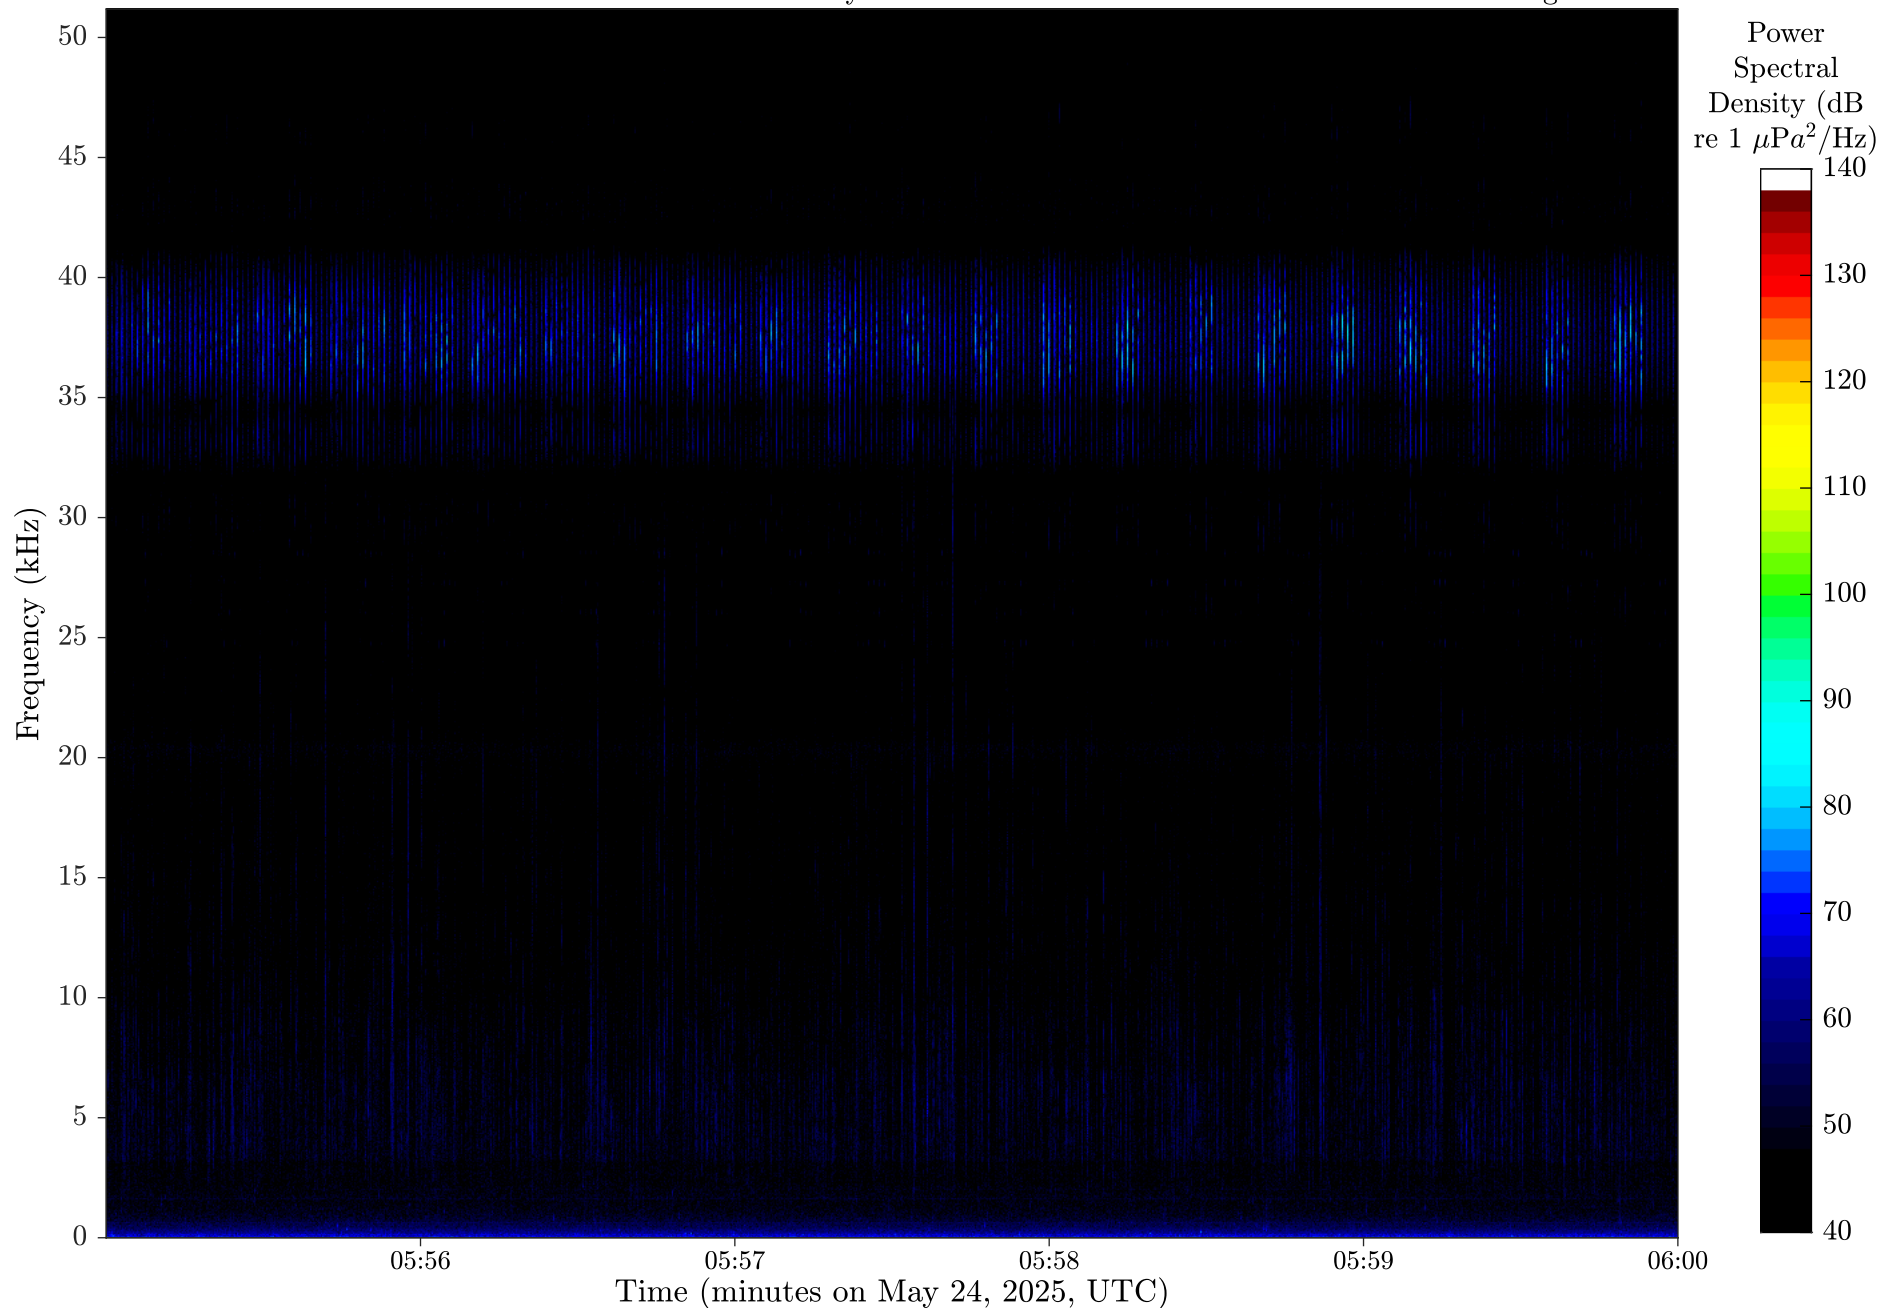


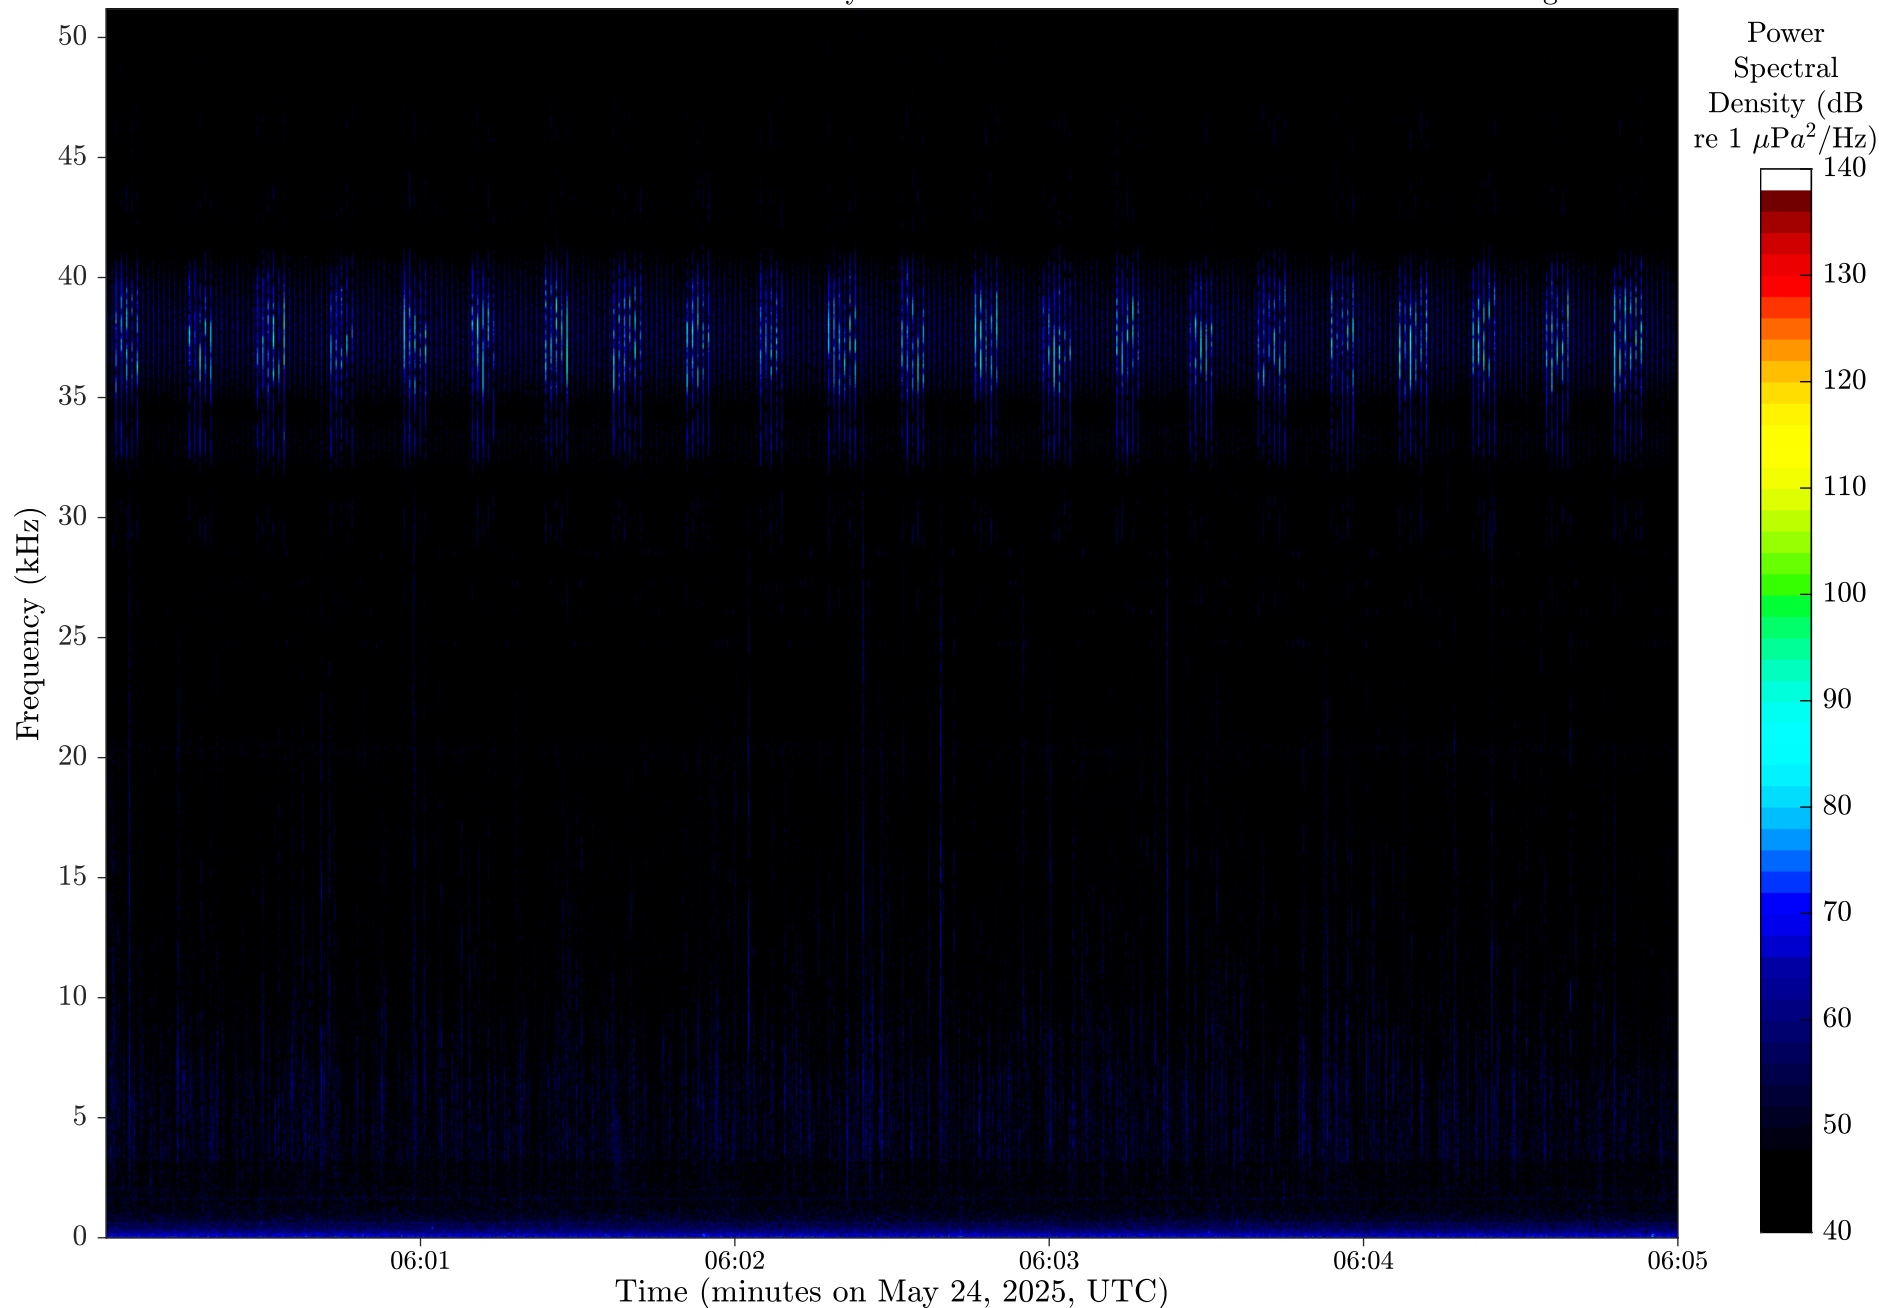

Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:21:00 UTC

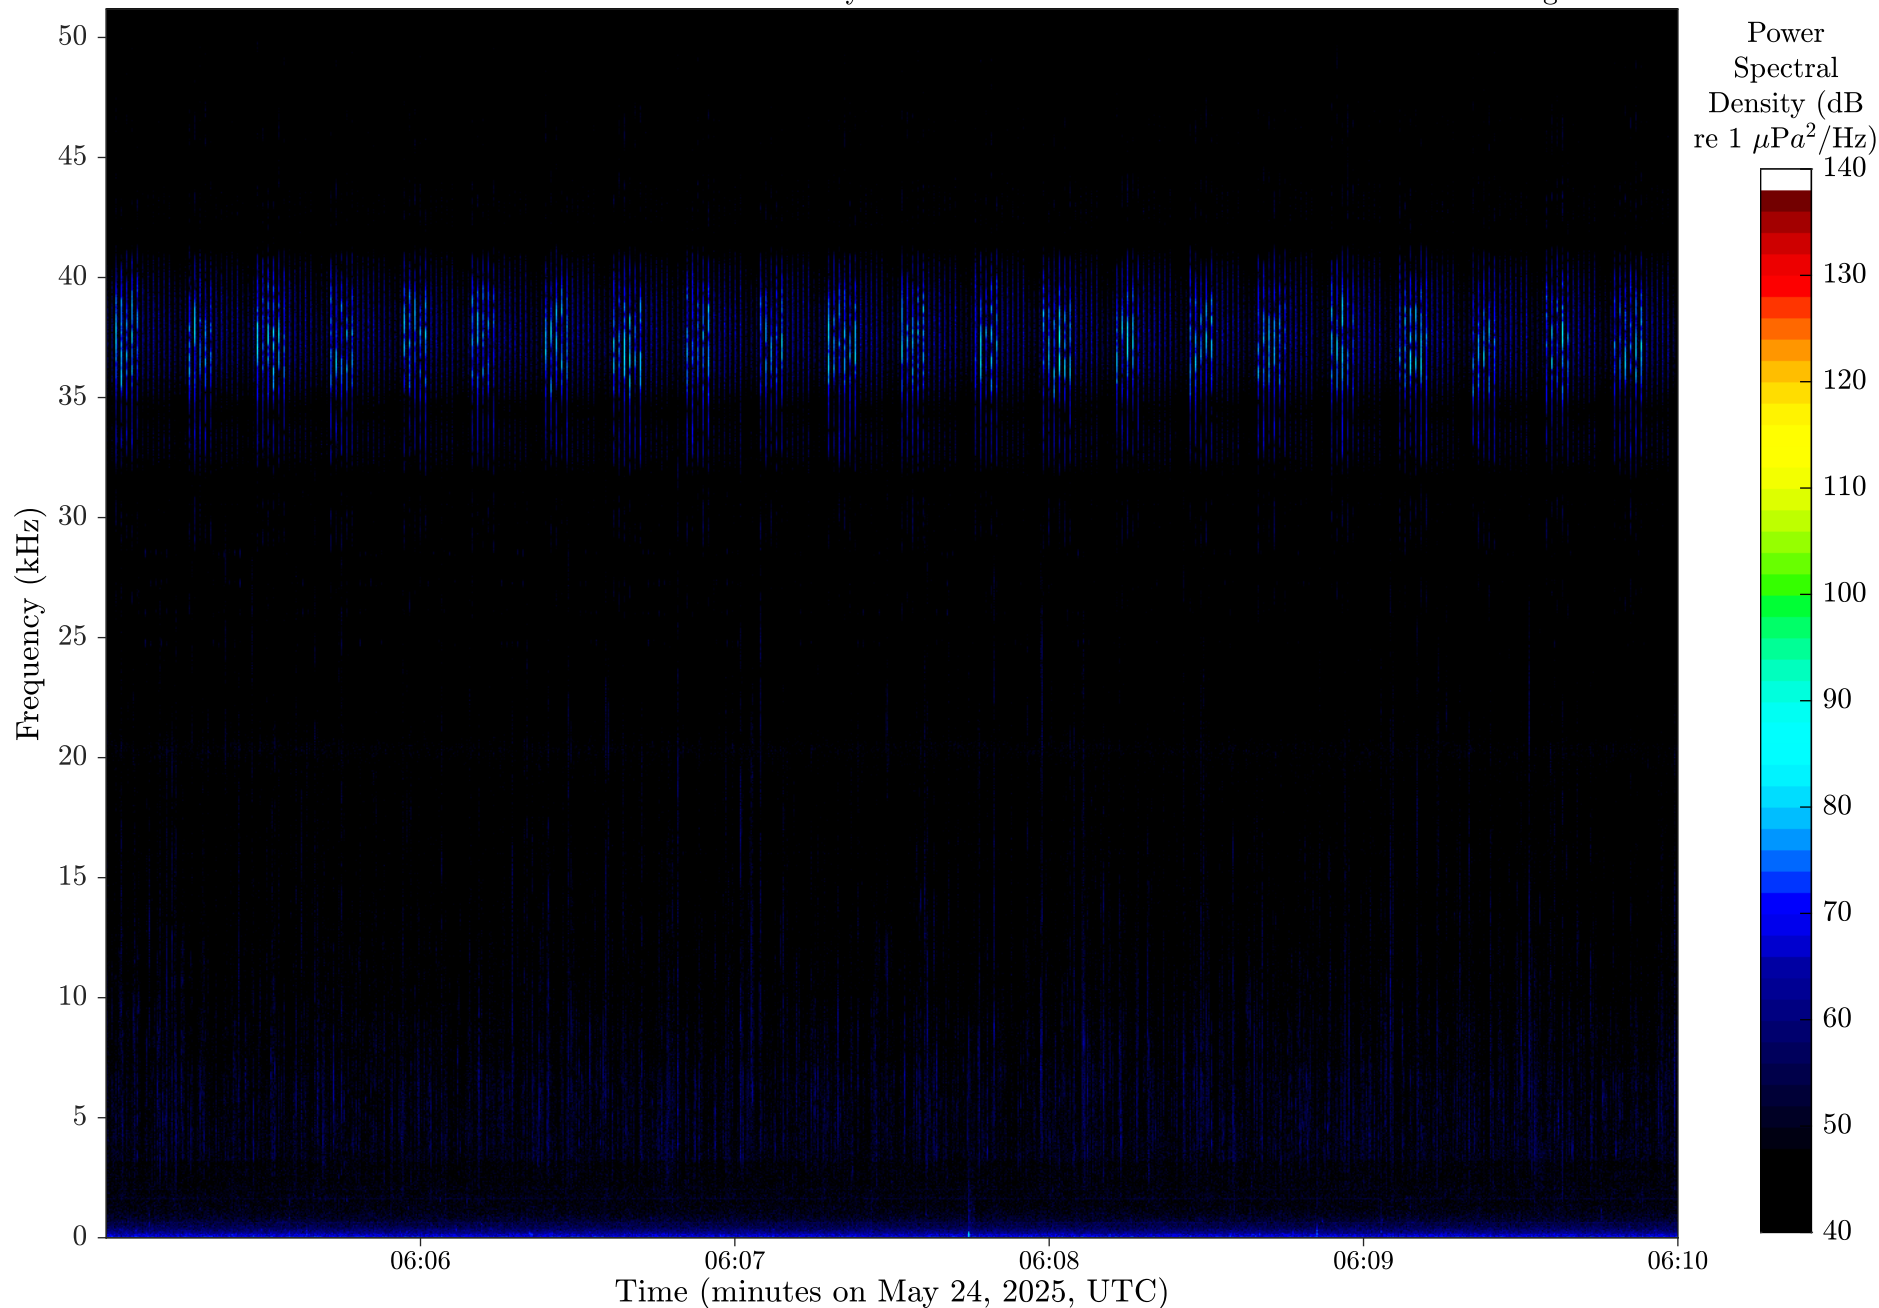

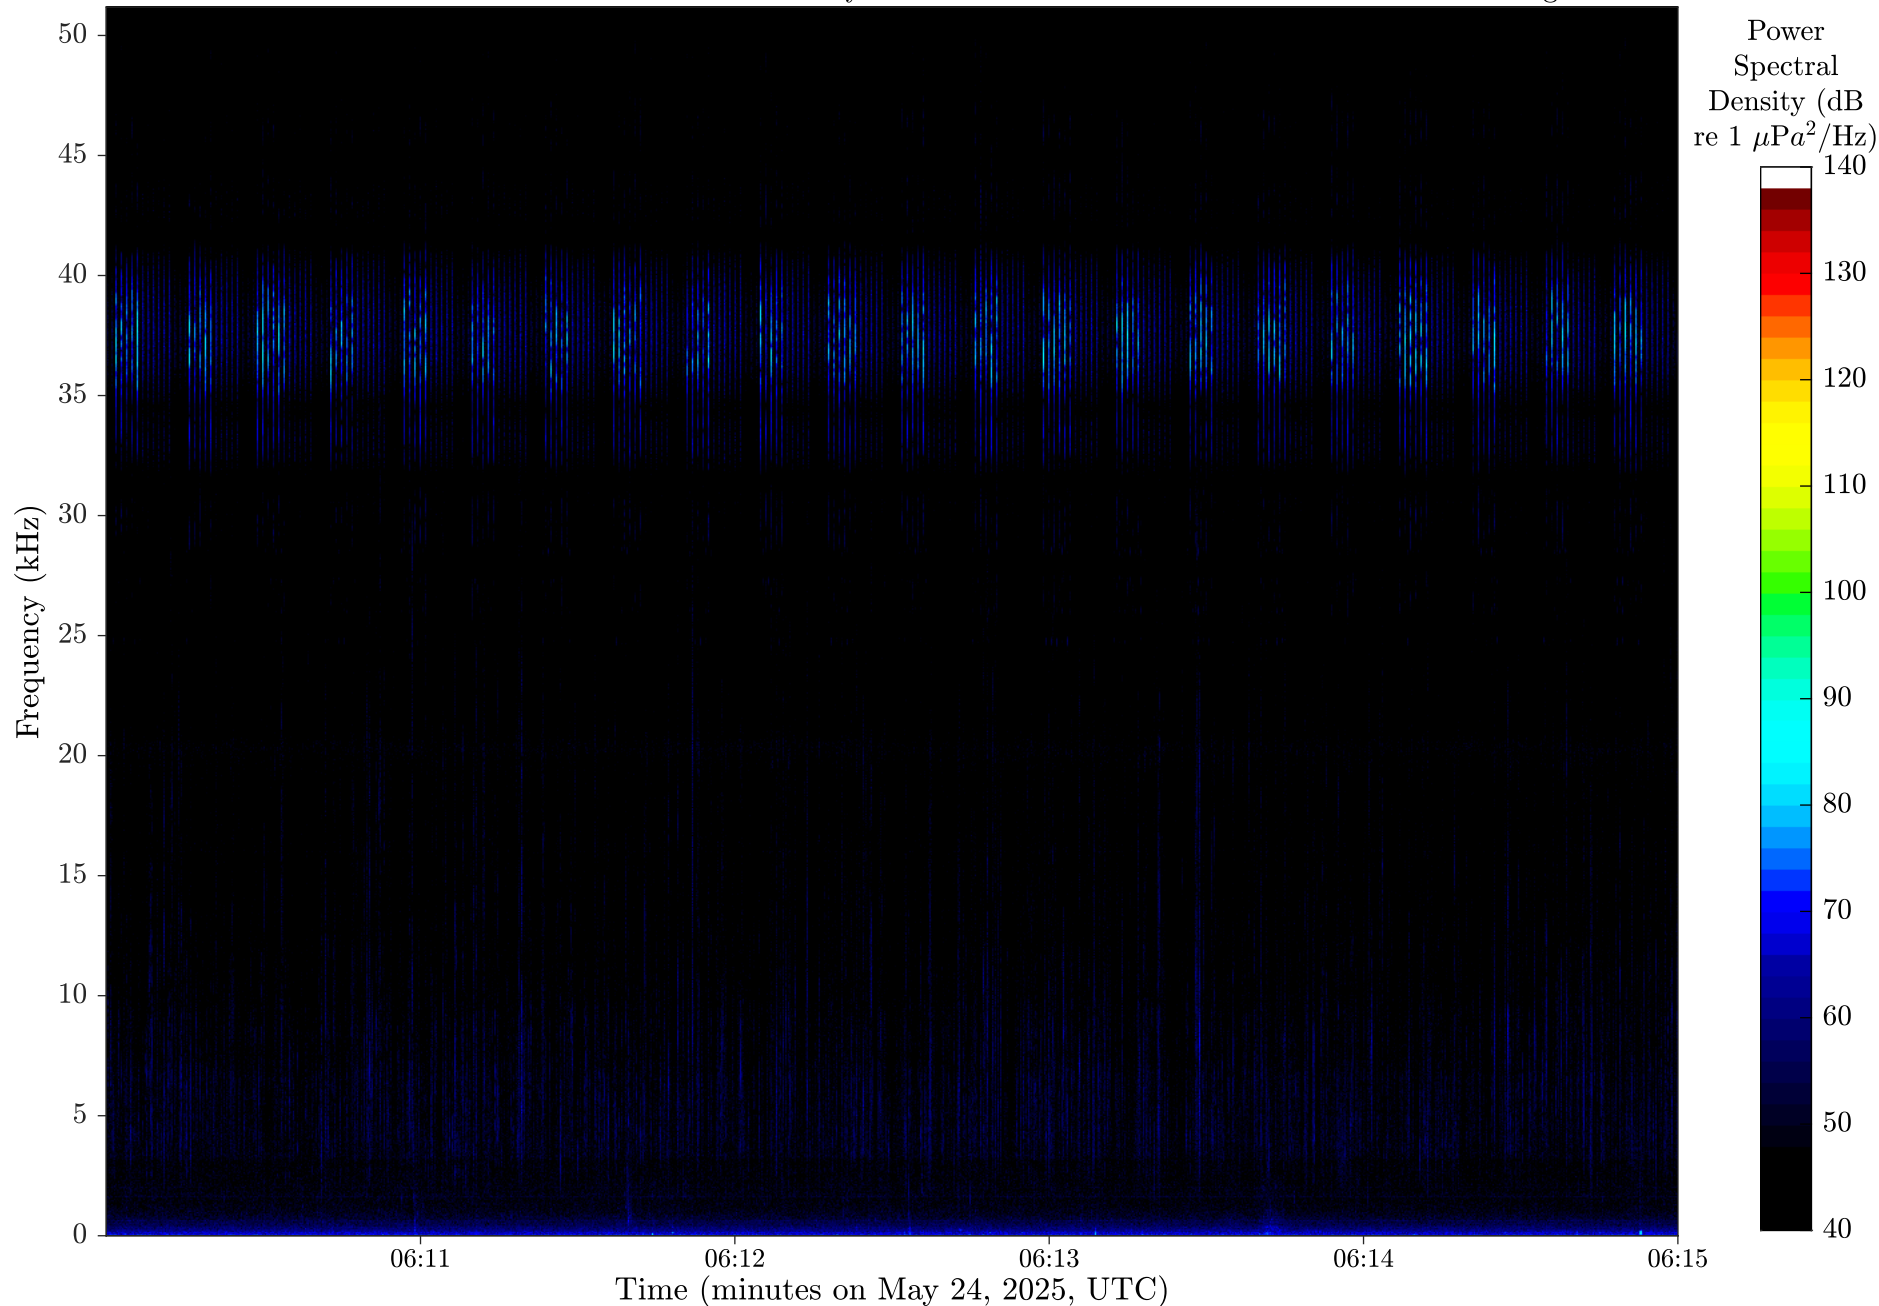


Comments: 36.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:14 UTC

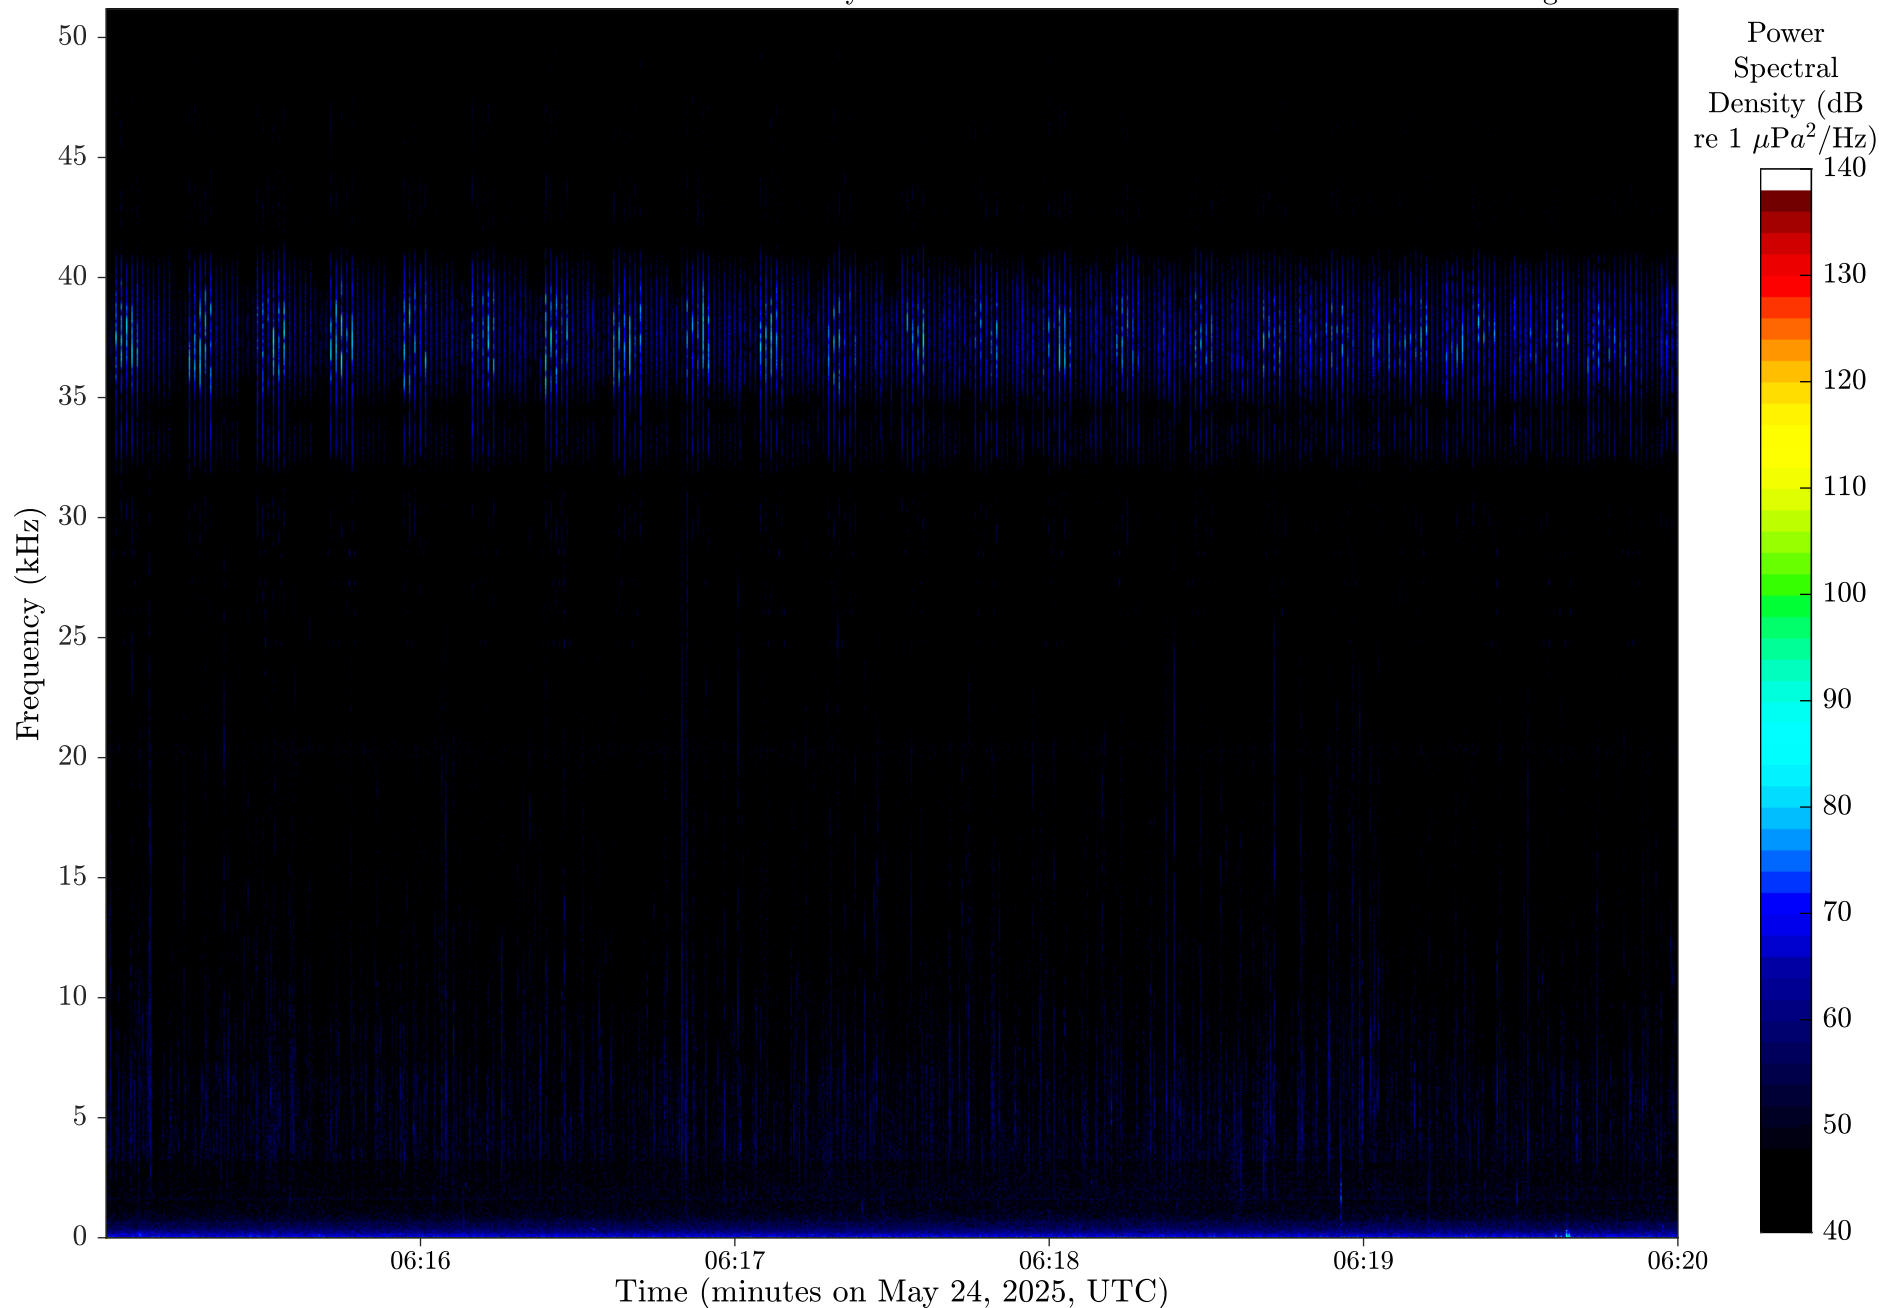


Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:21:21 UTC

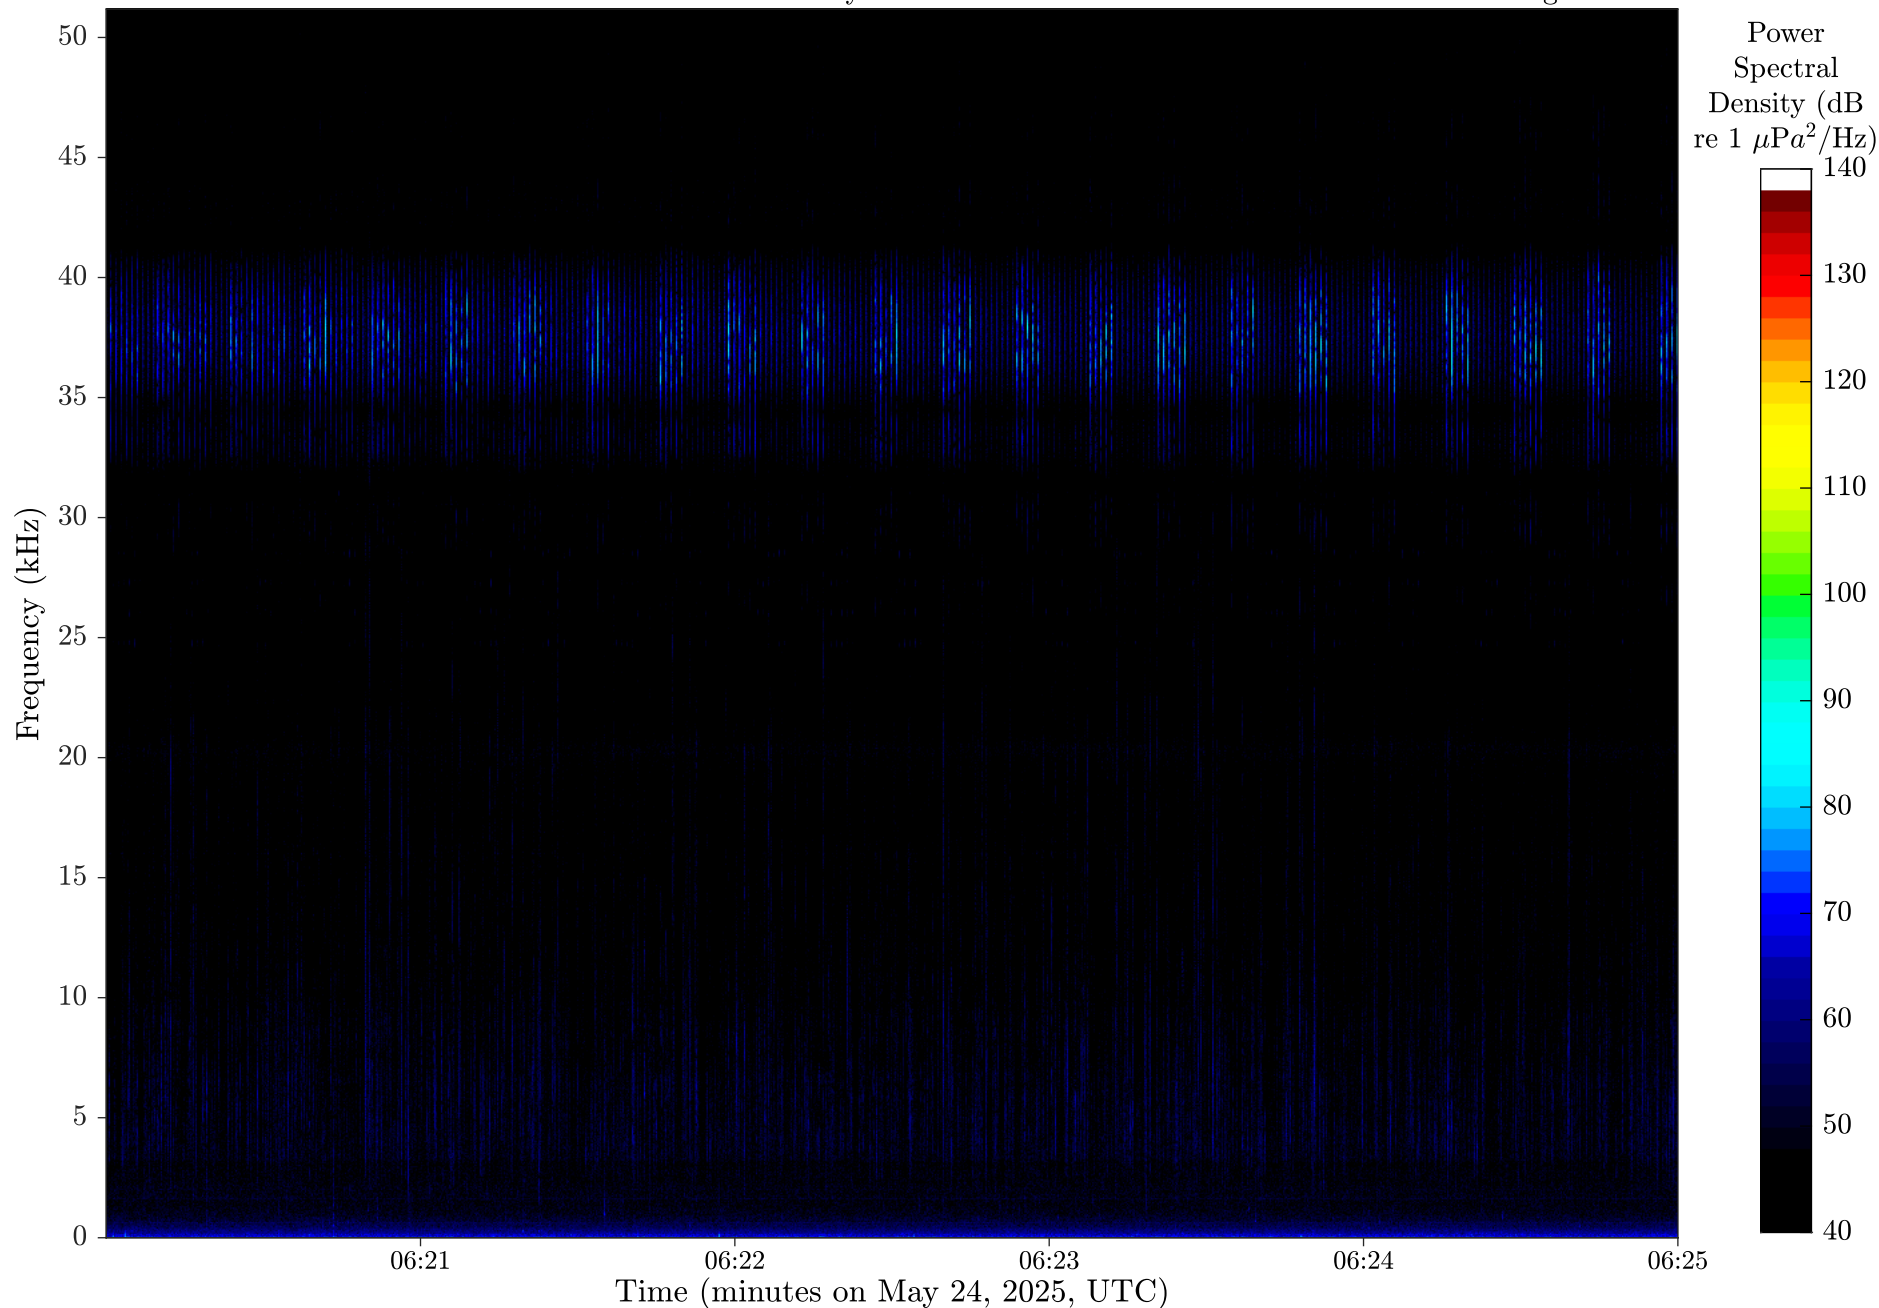


Comments: 35.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:28 UTC

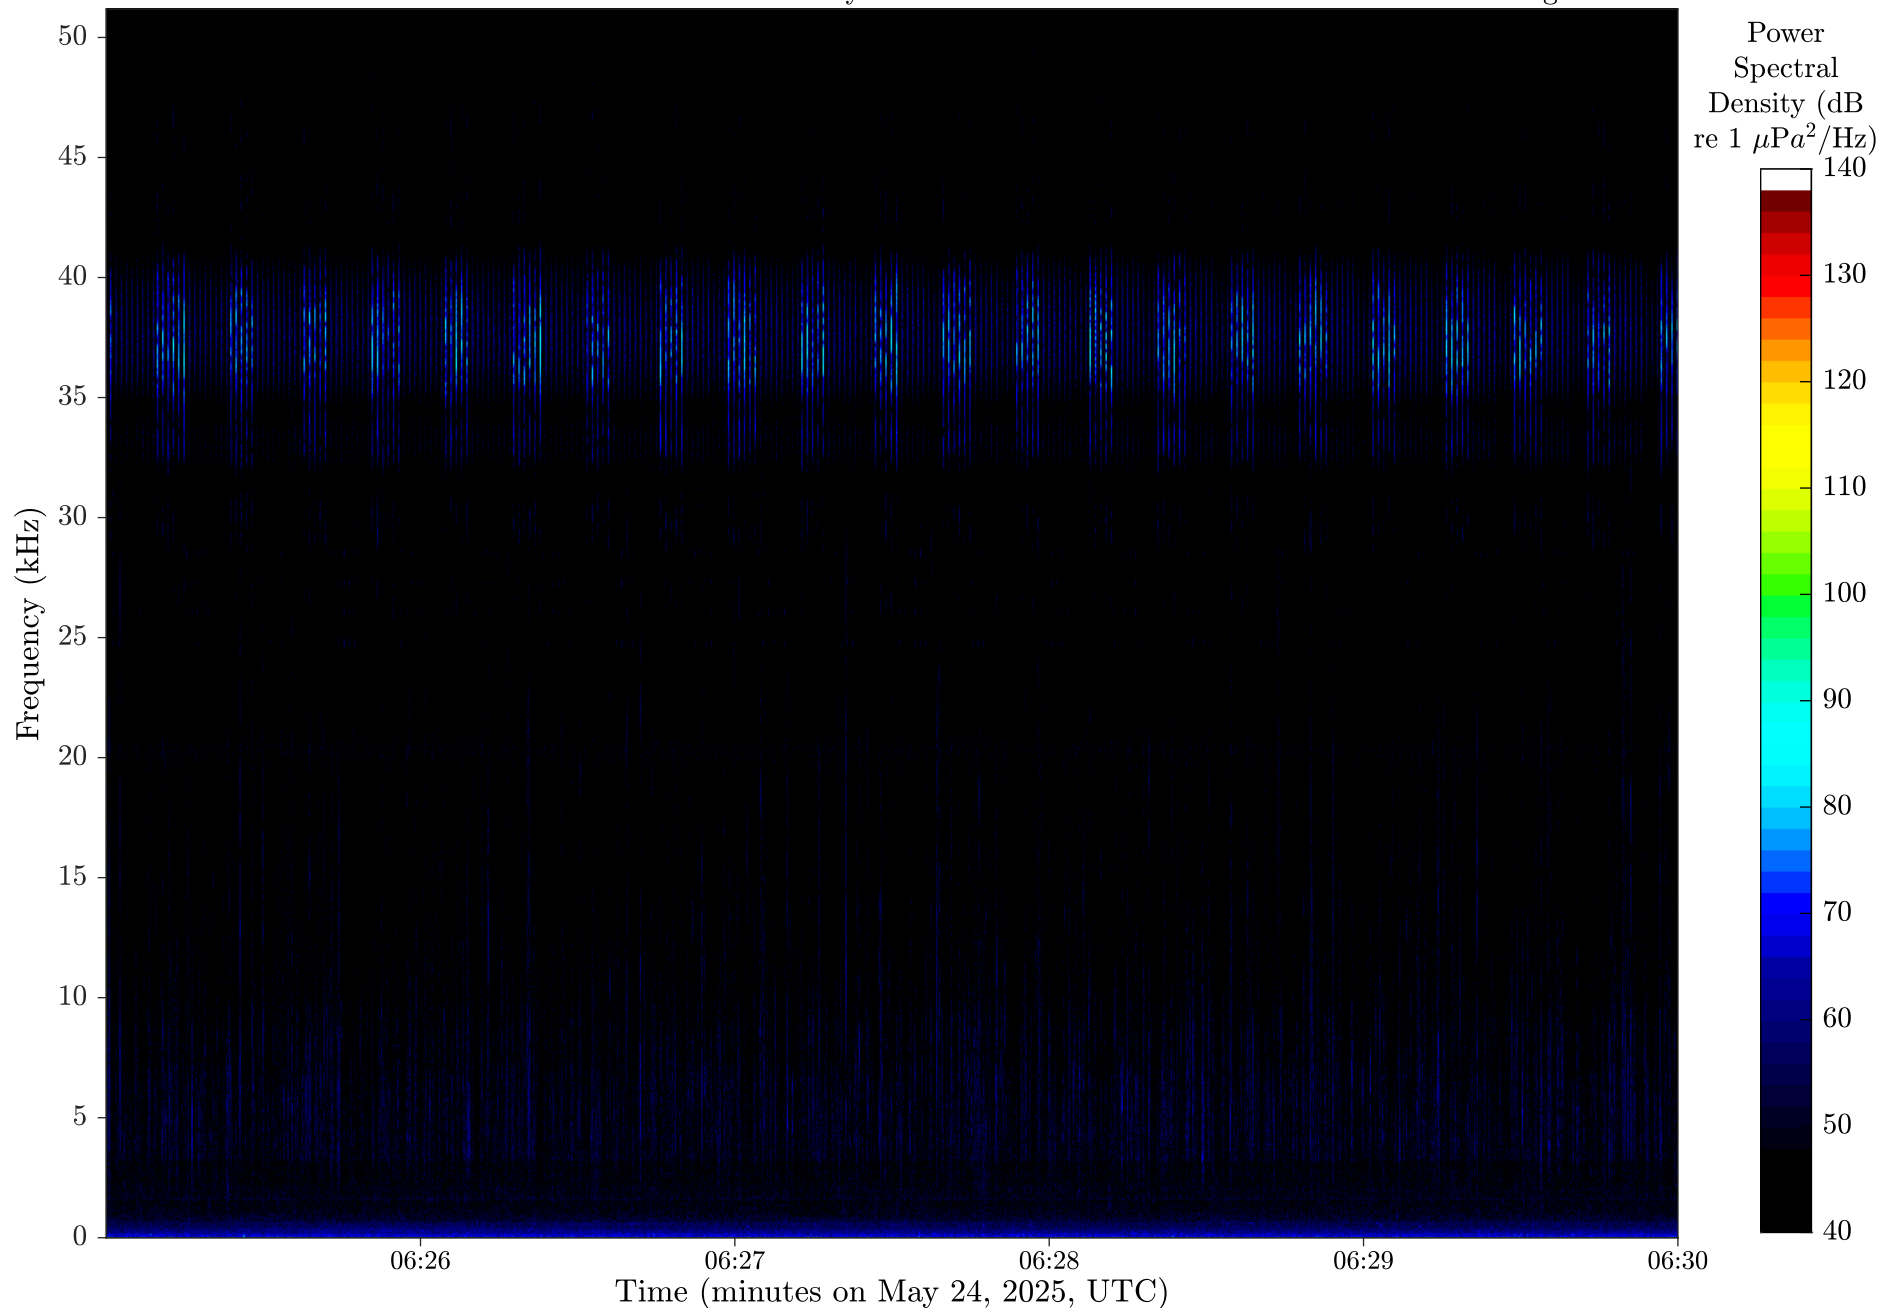


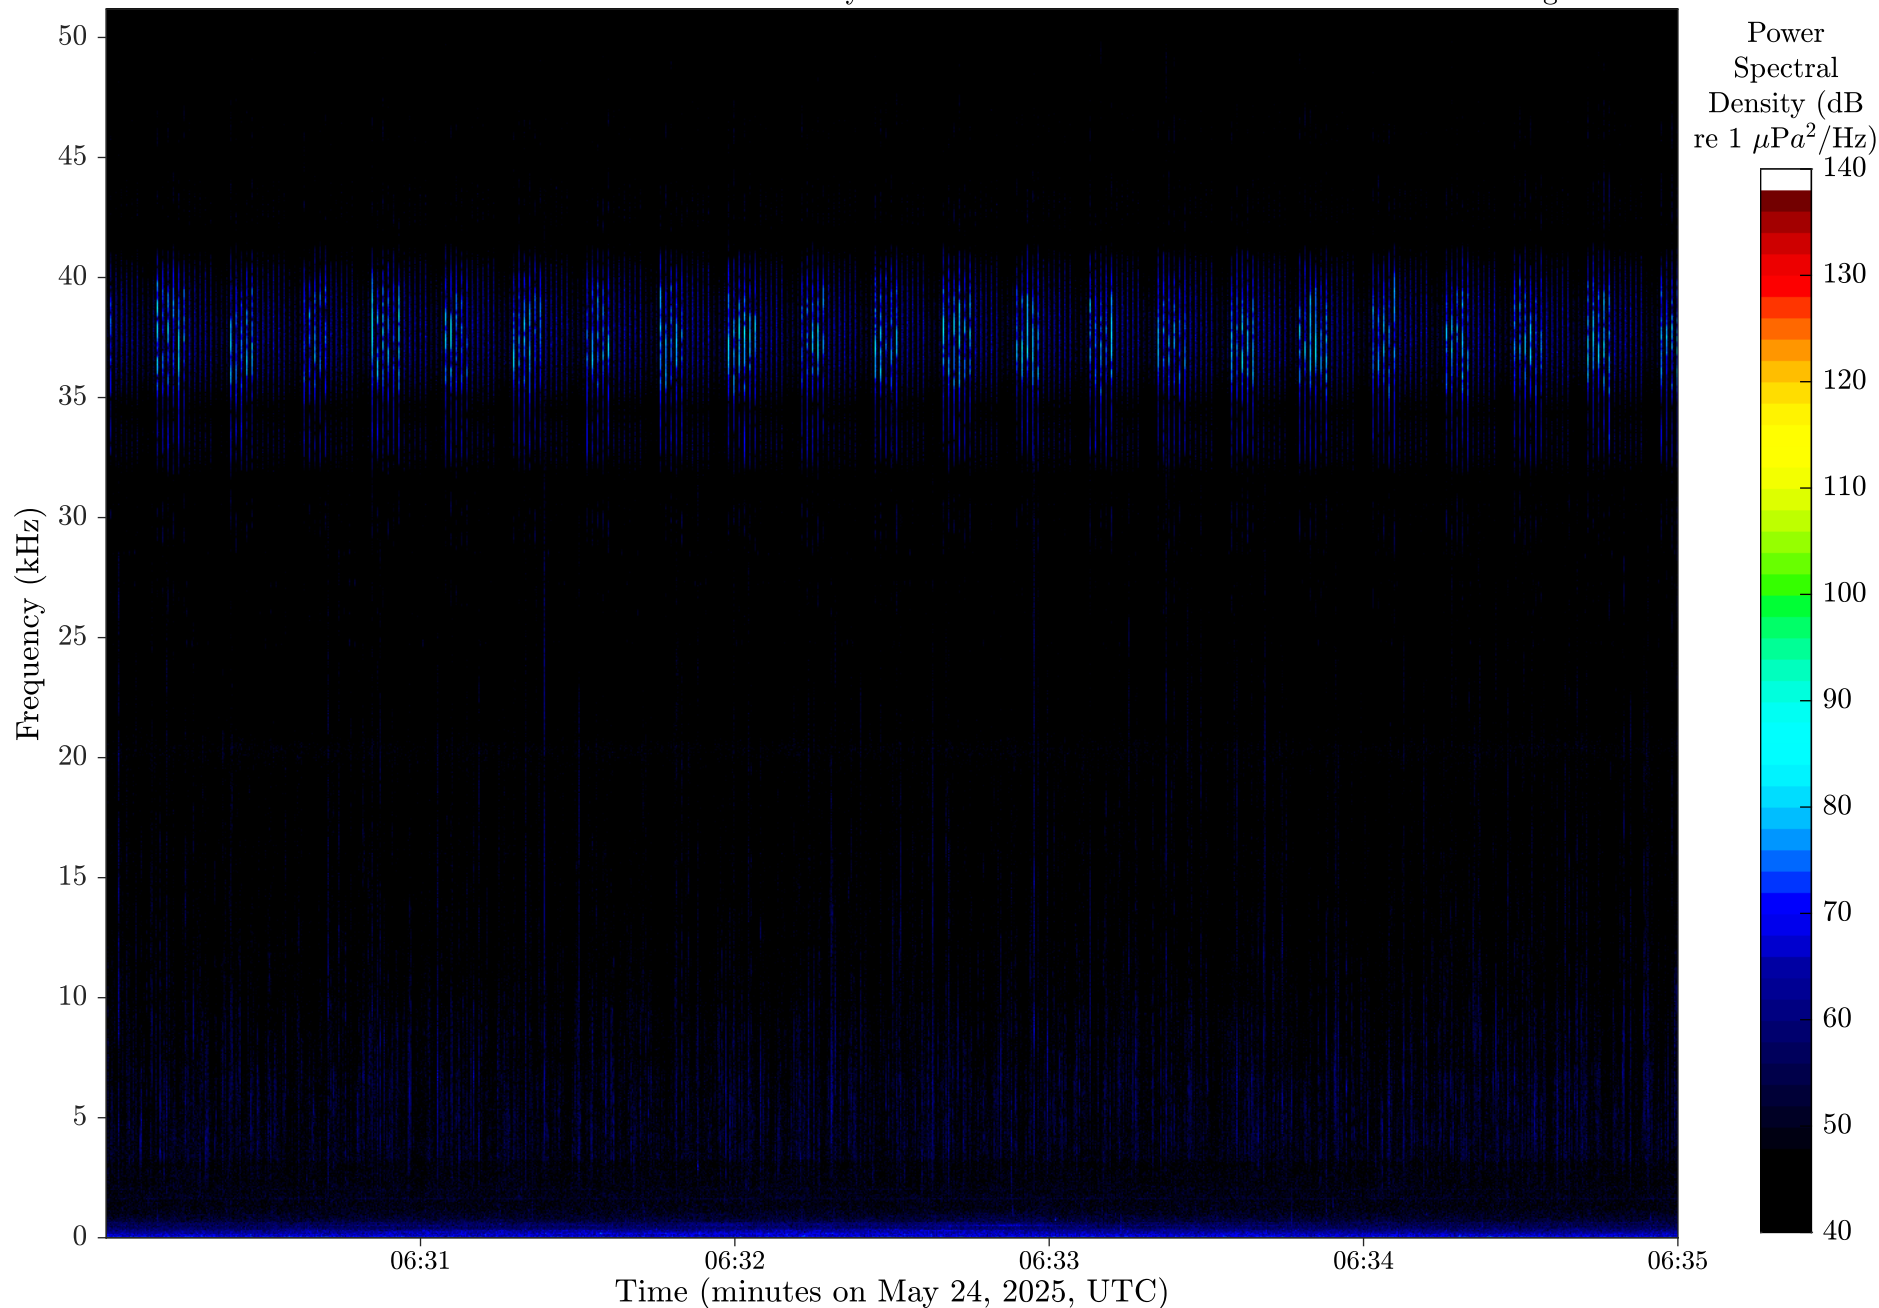


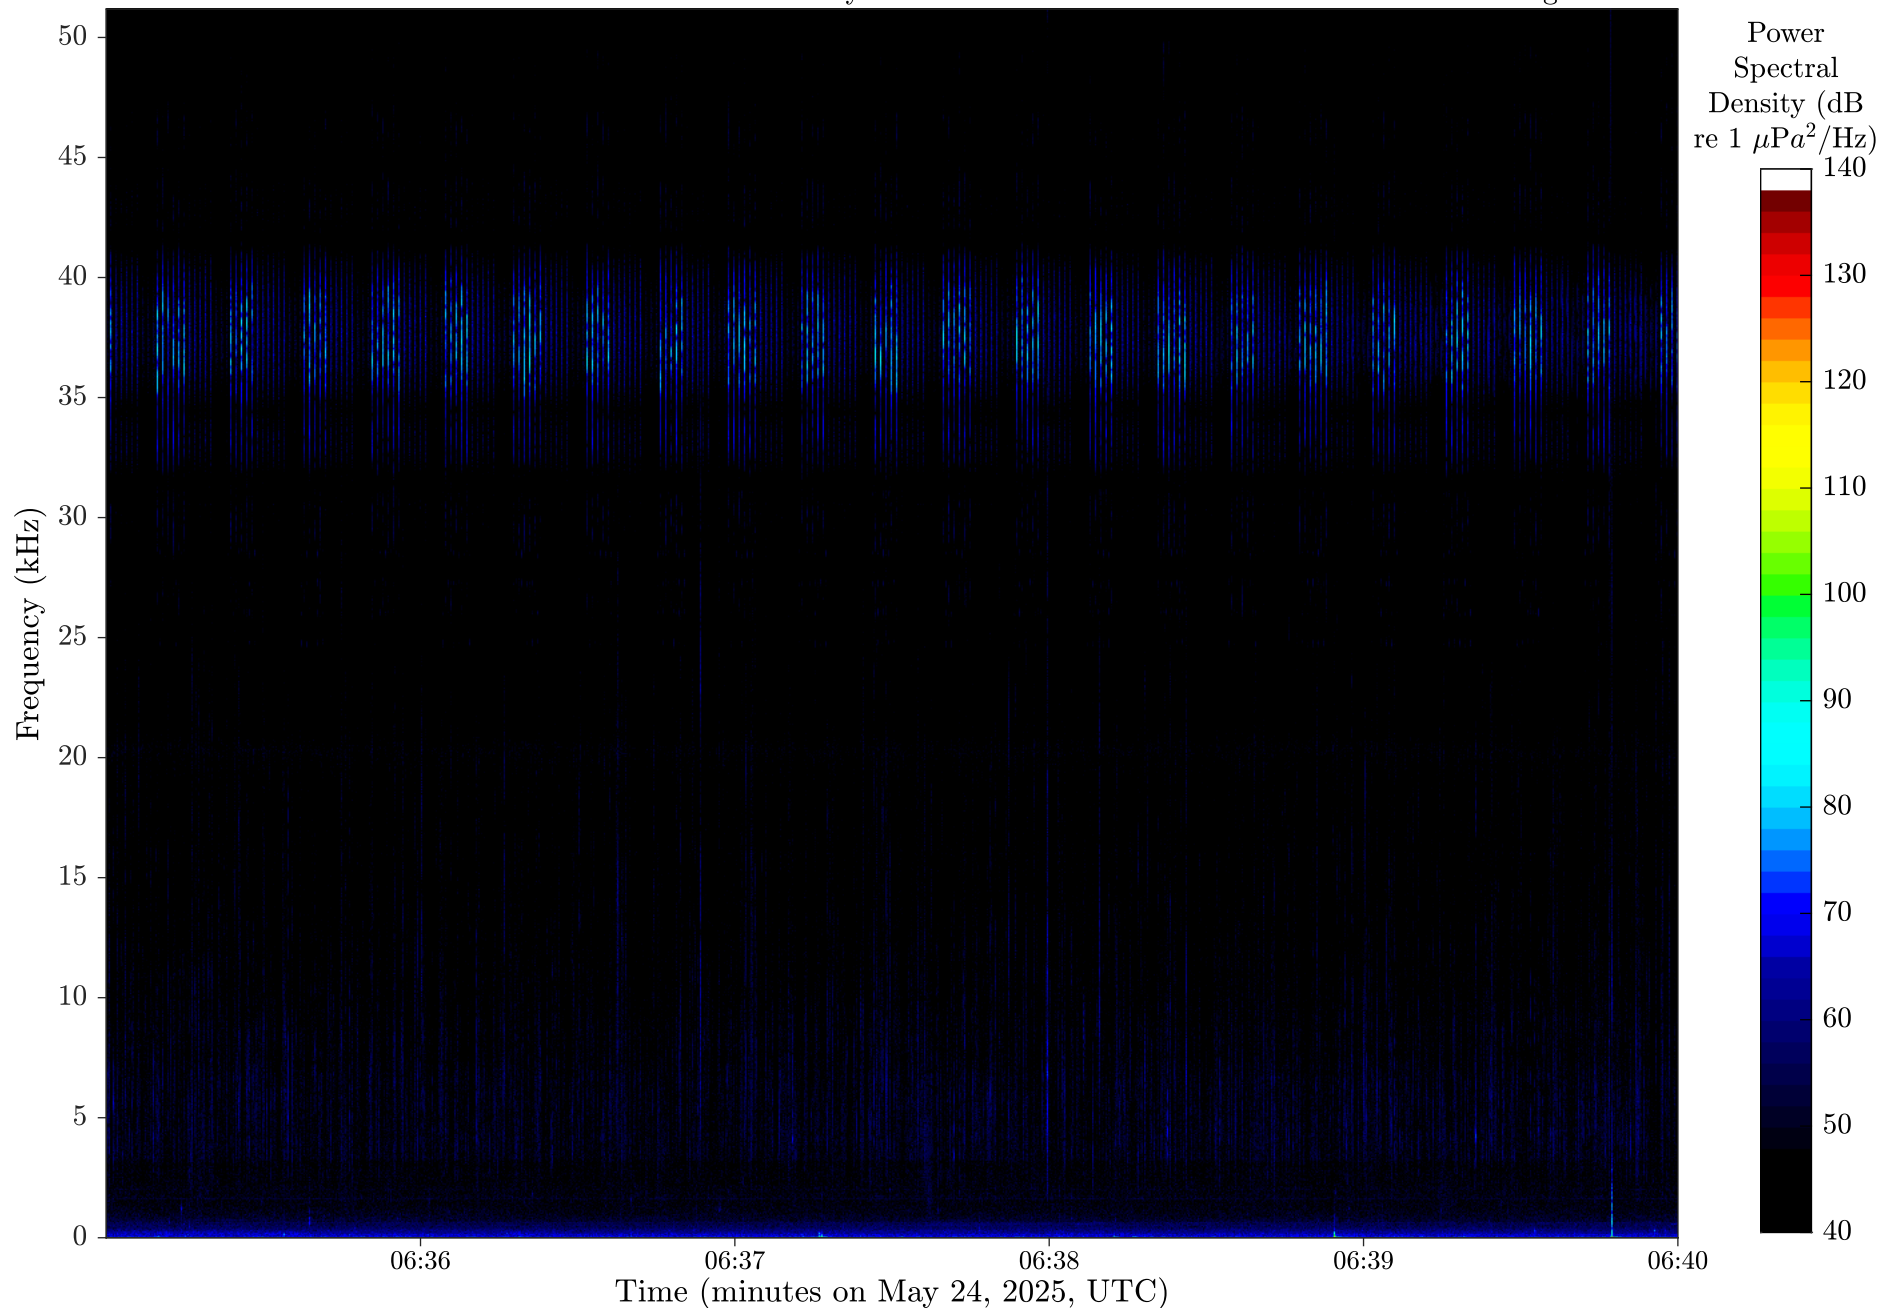

Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:21:50 UTC

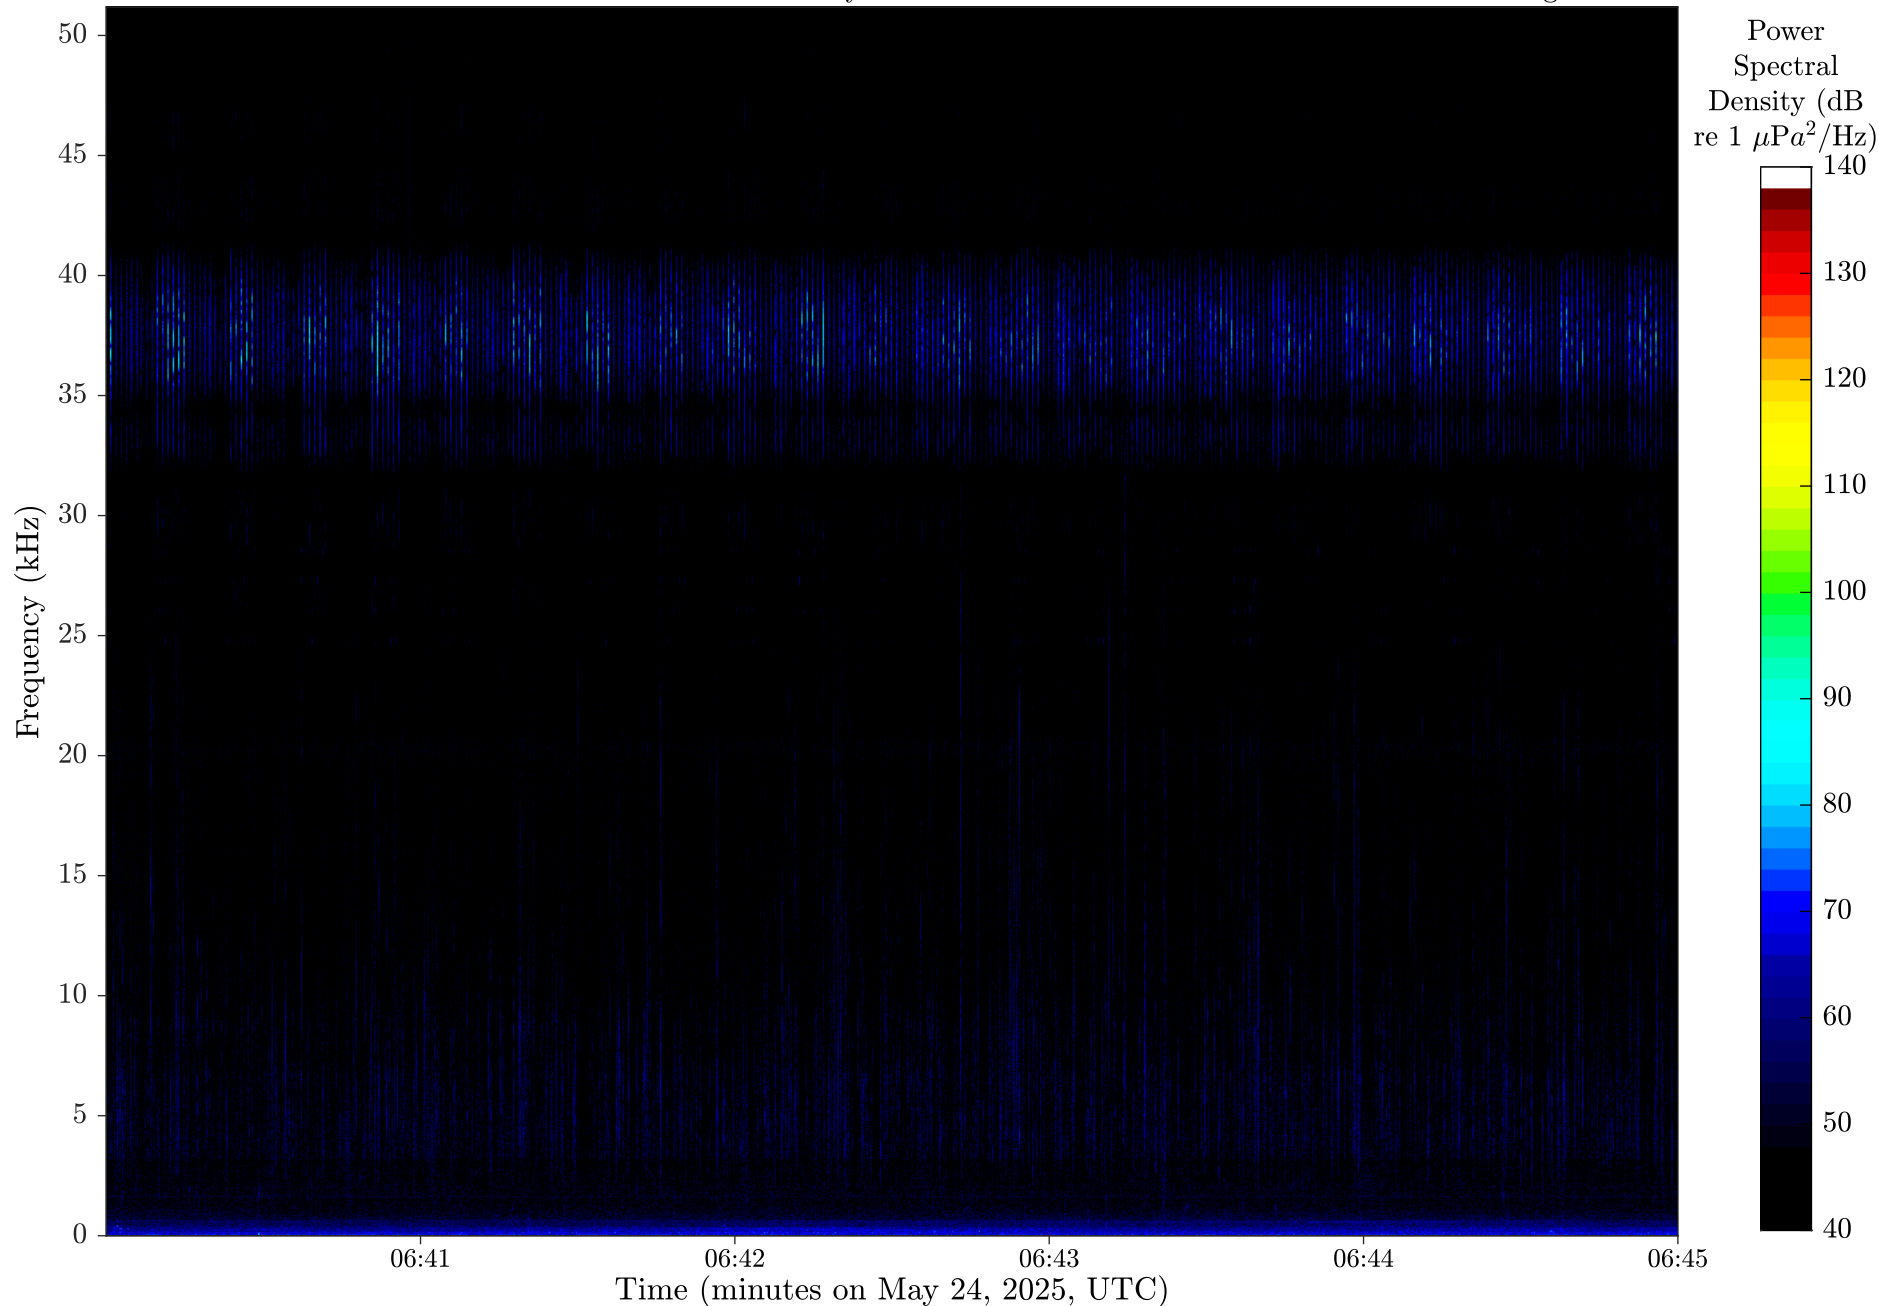


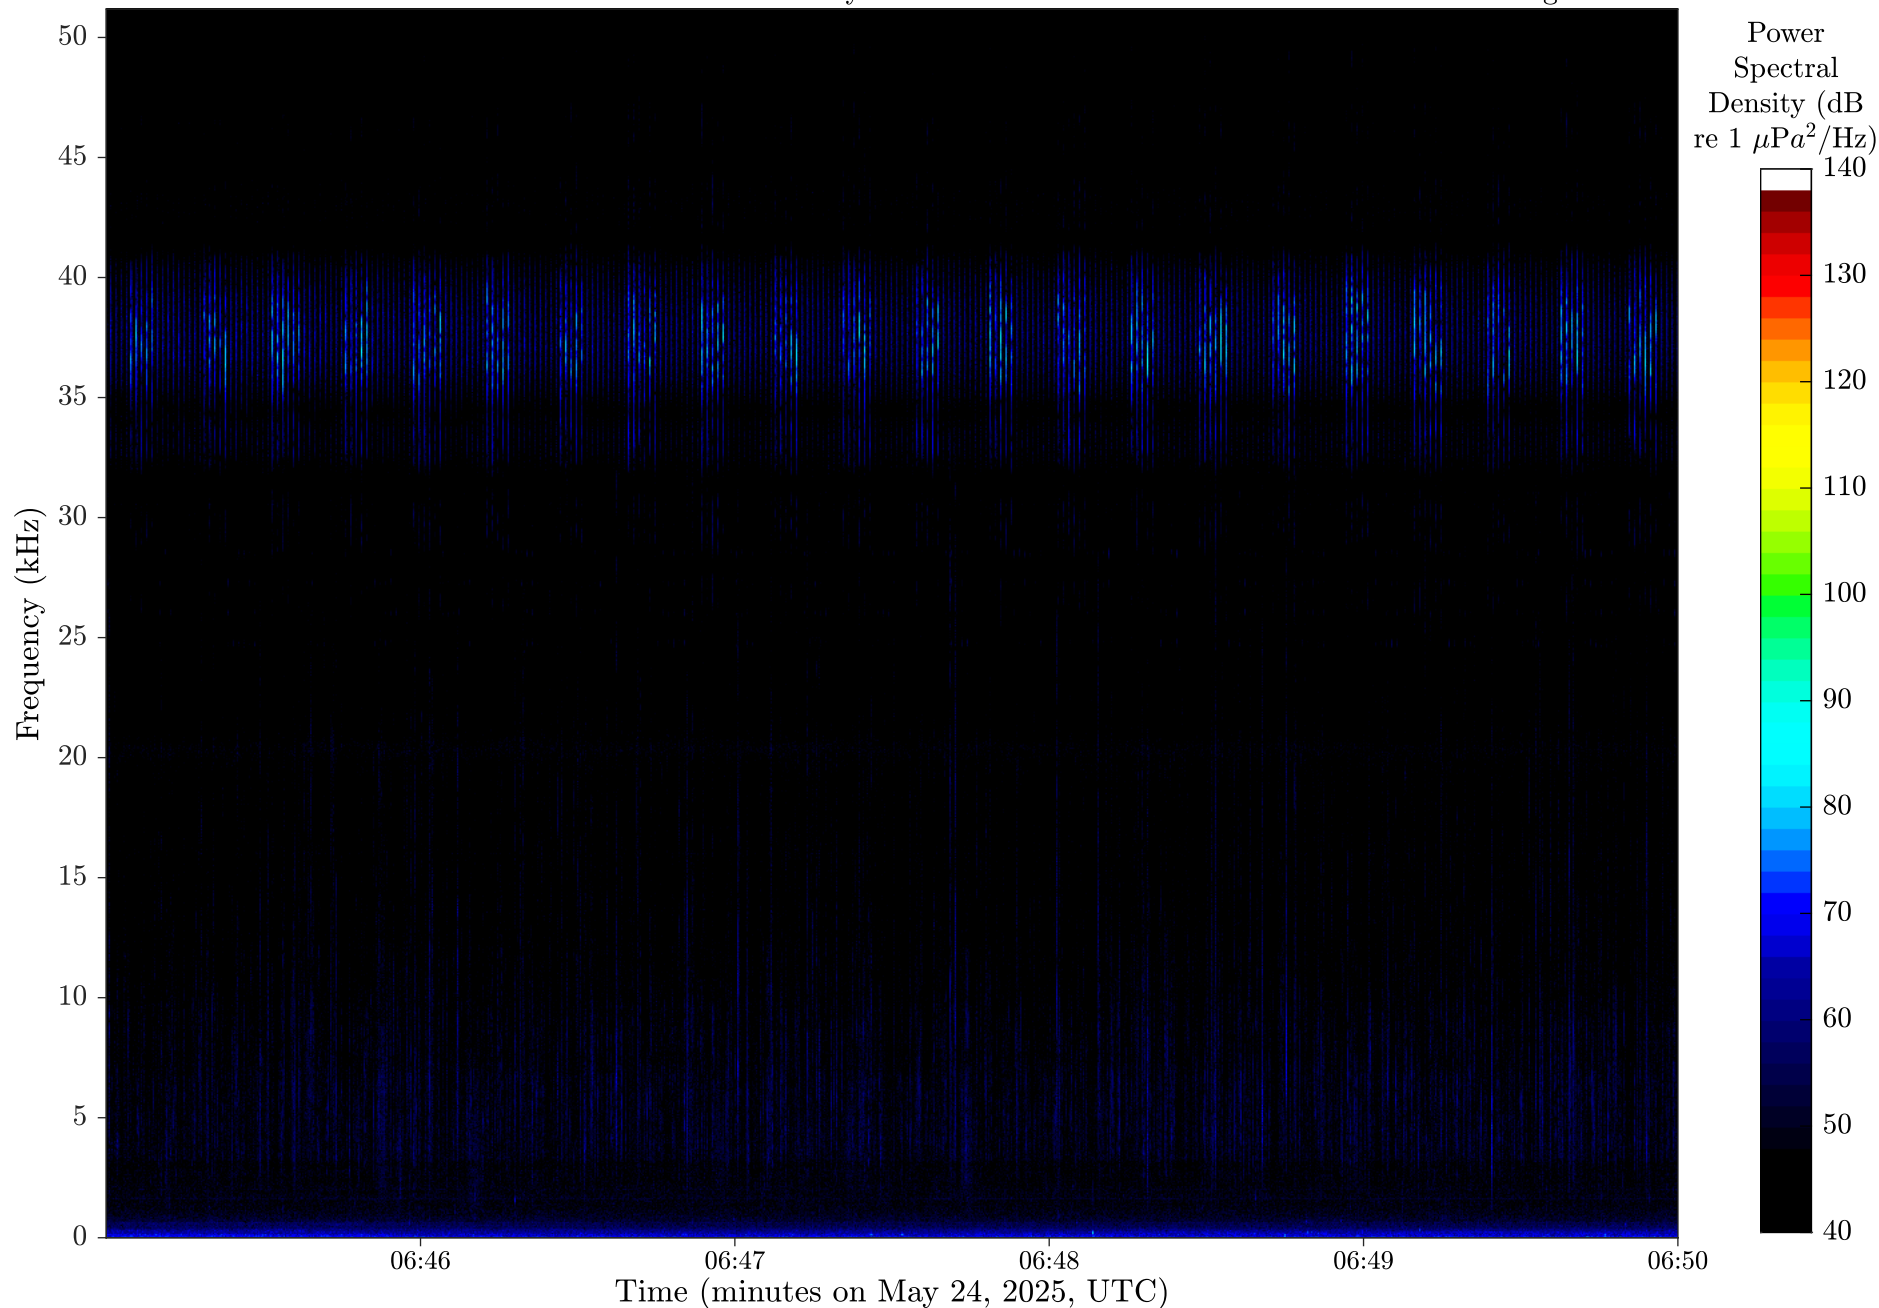

Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:22:03 UTC

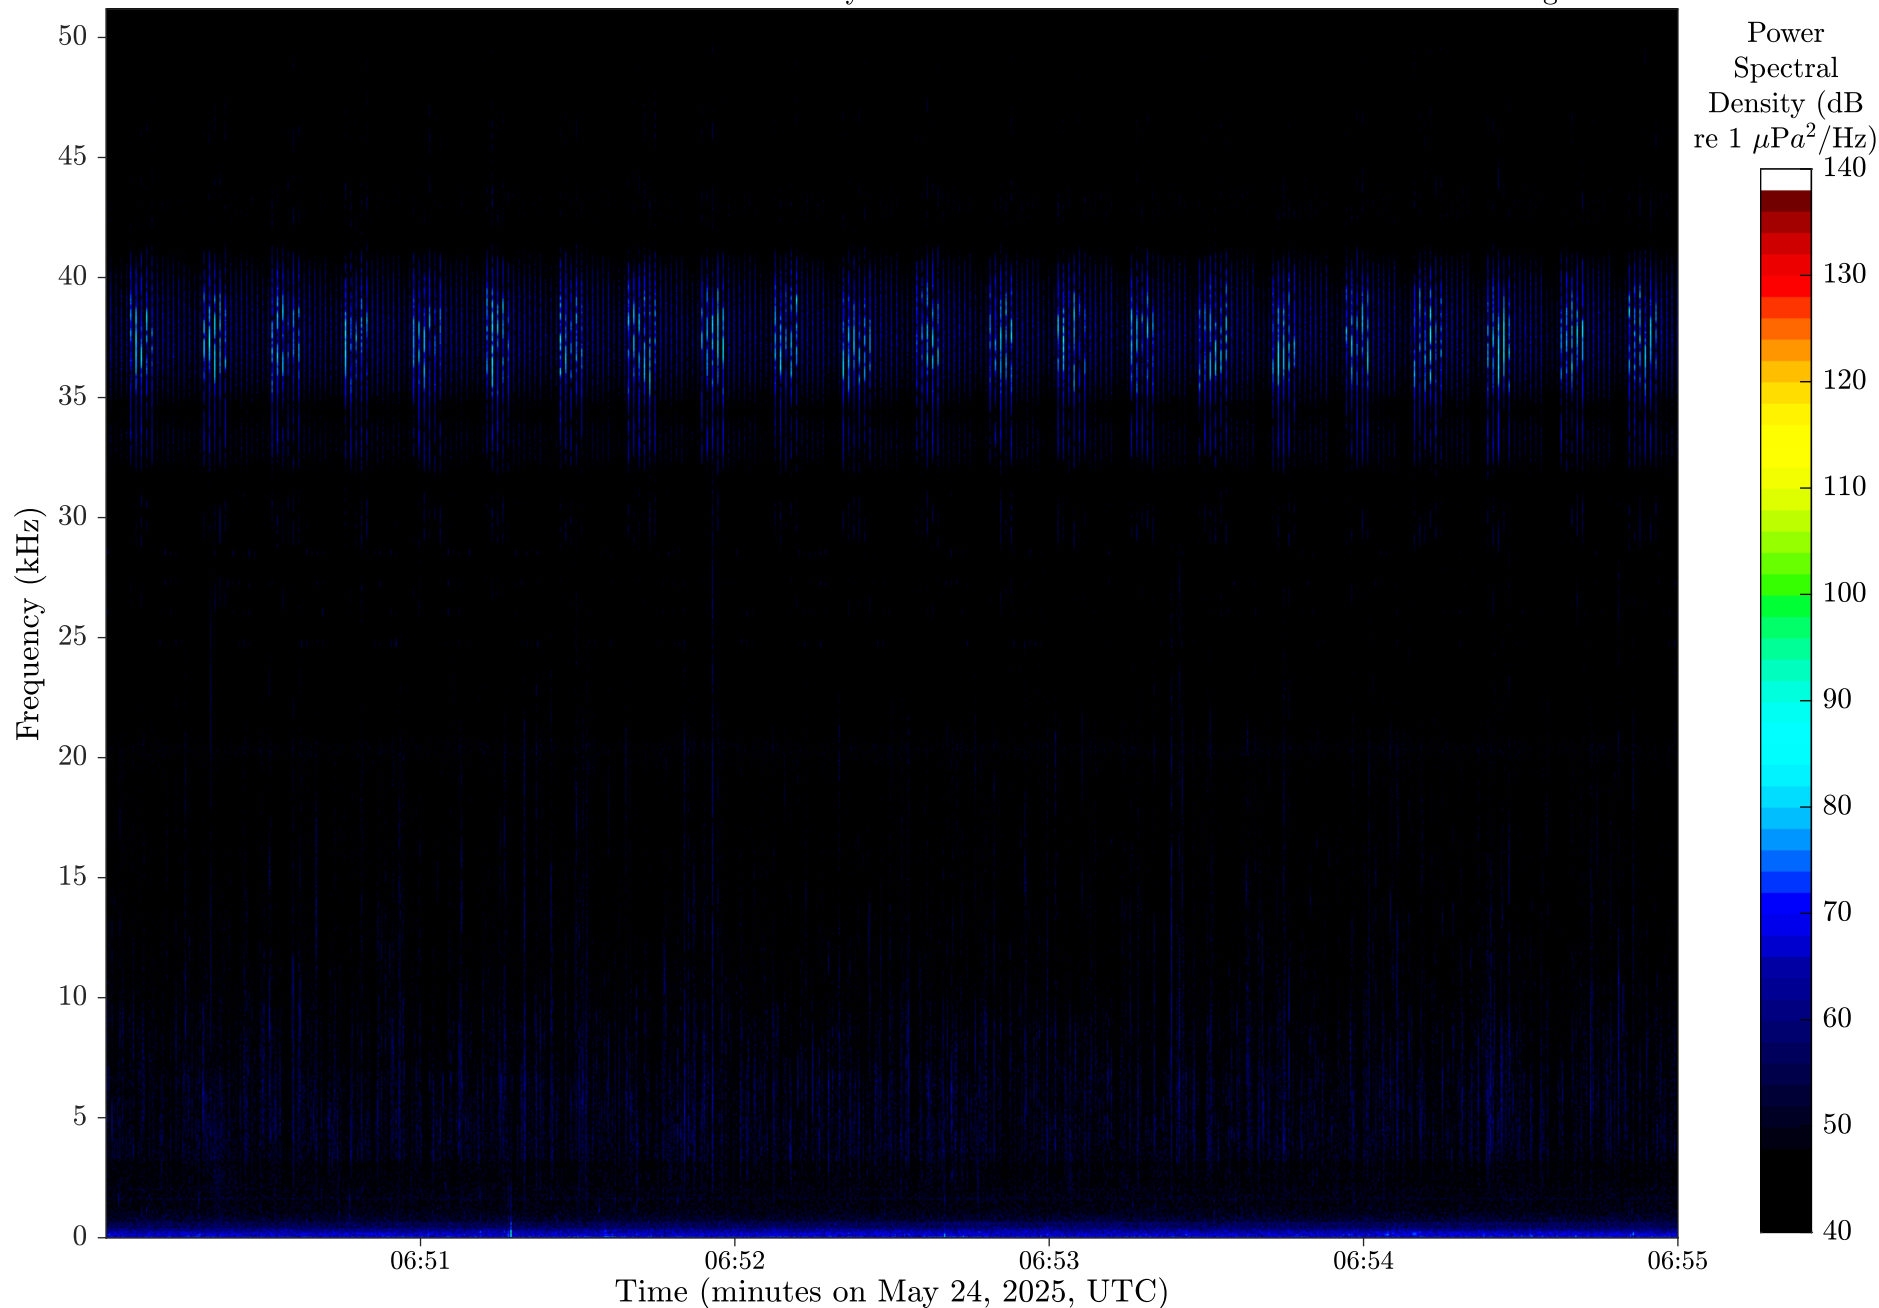


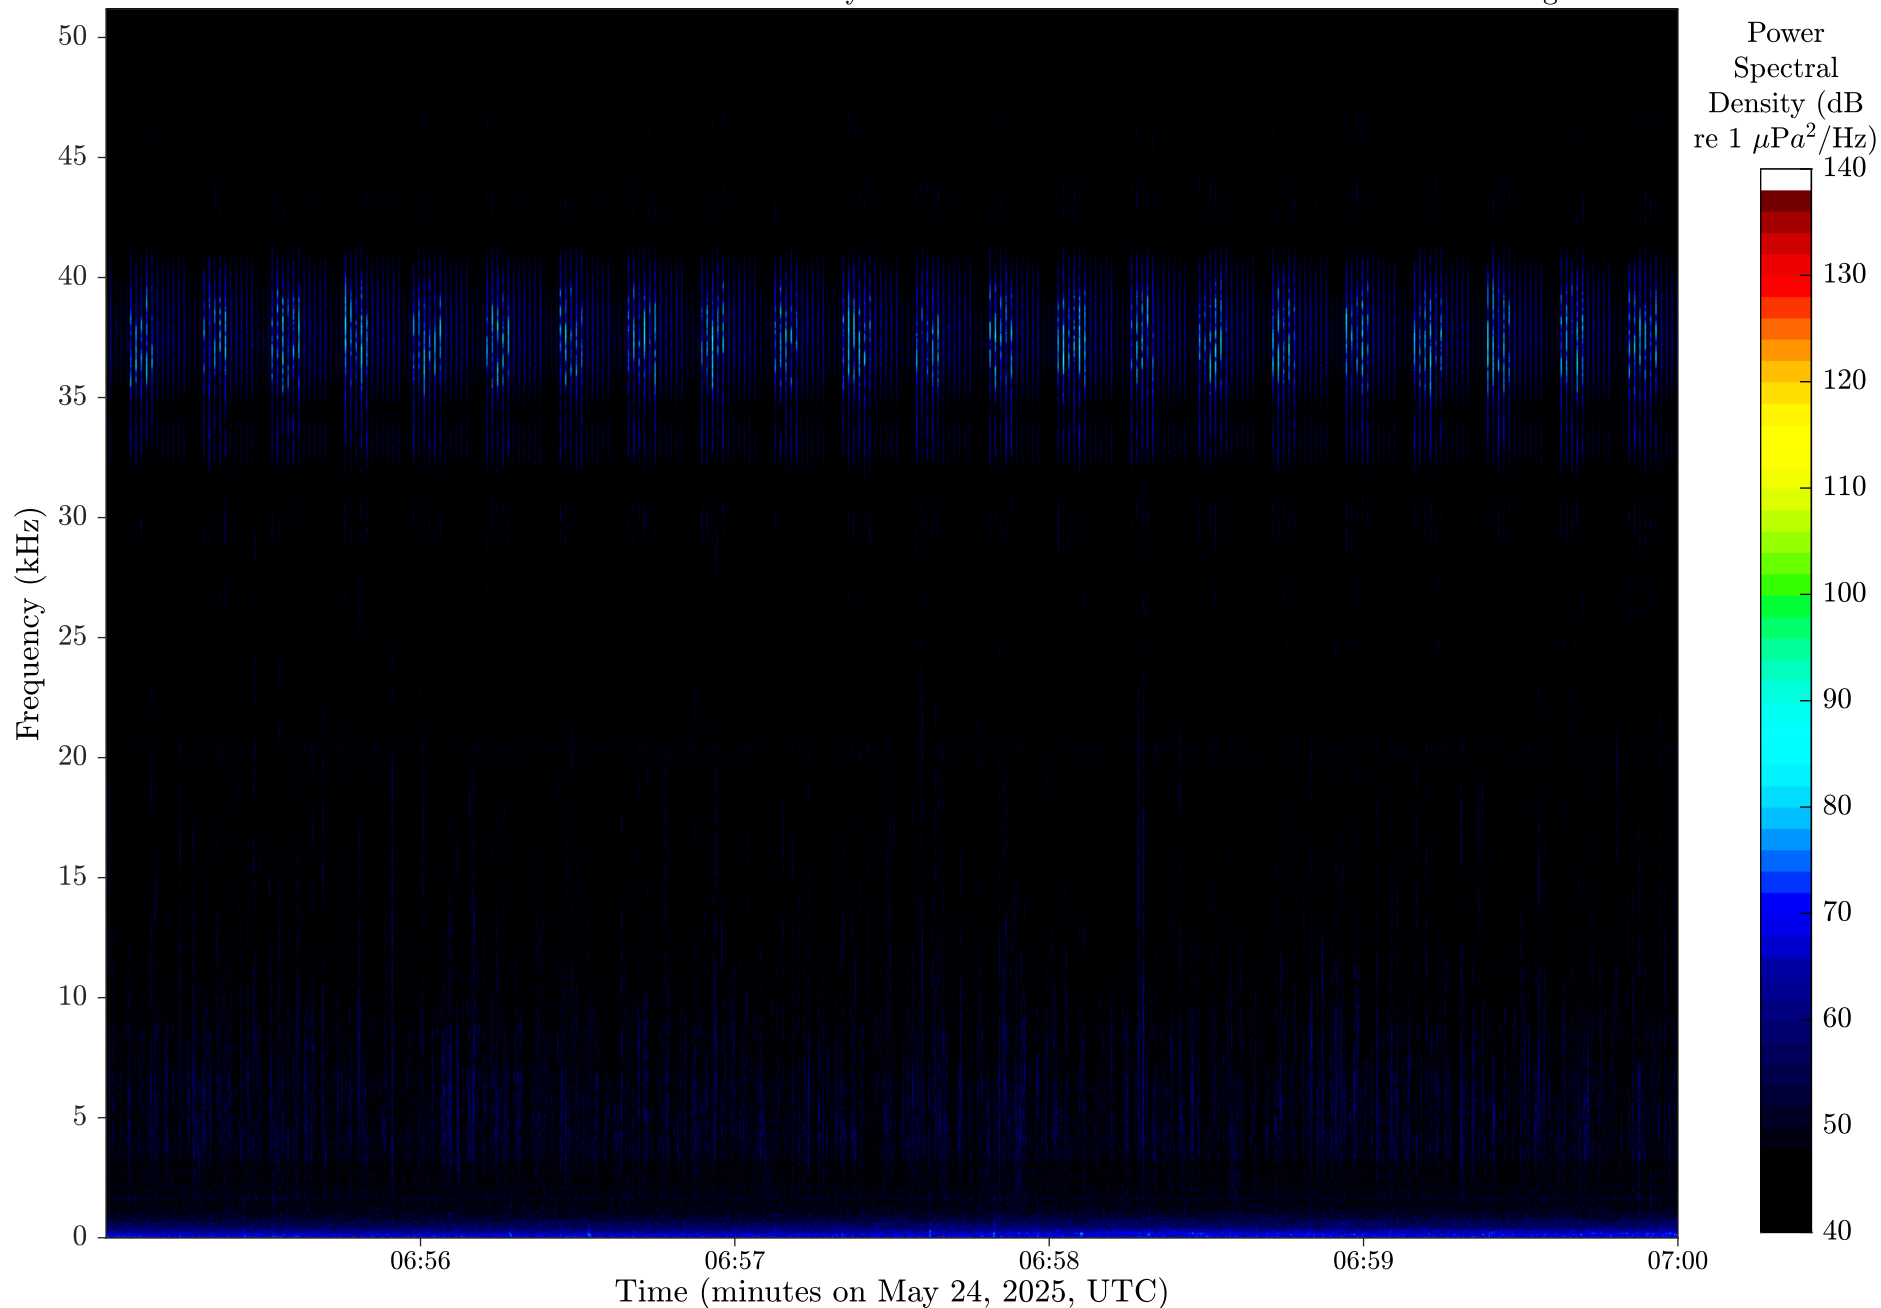


Comments: 36.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:19 UTC

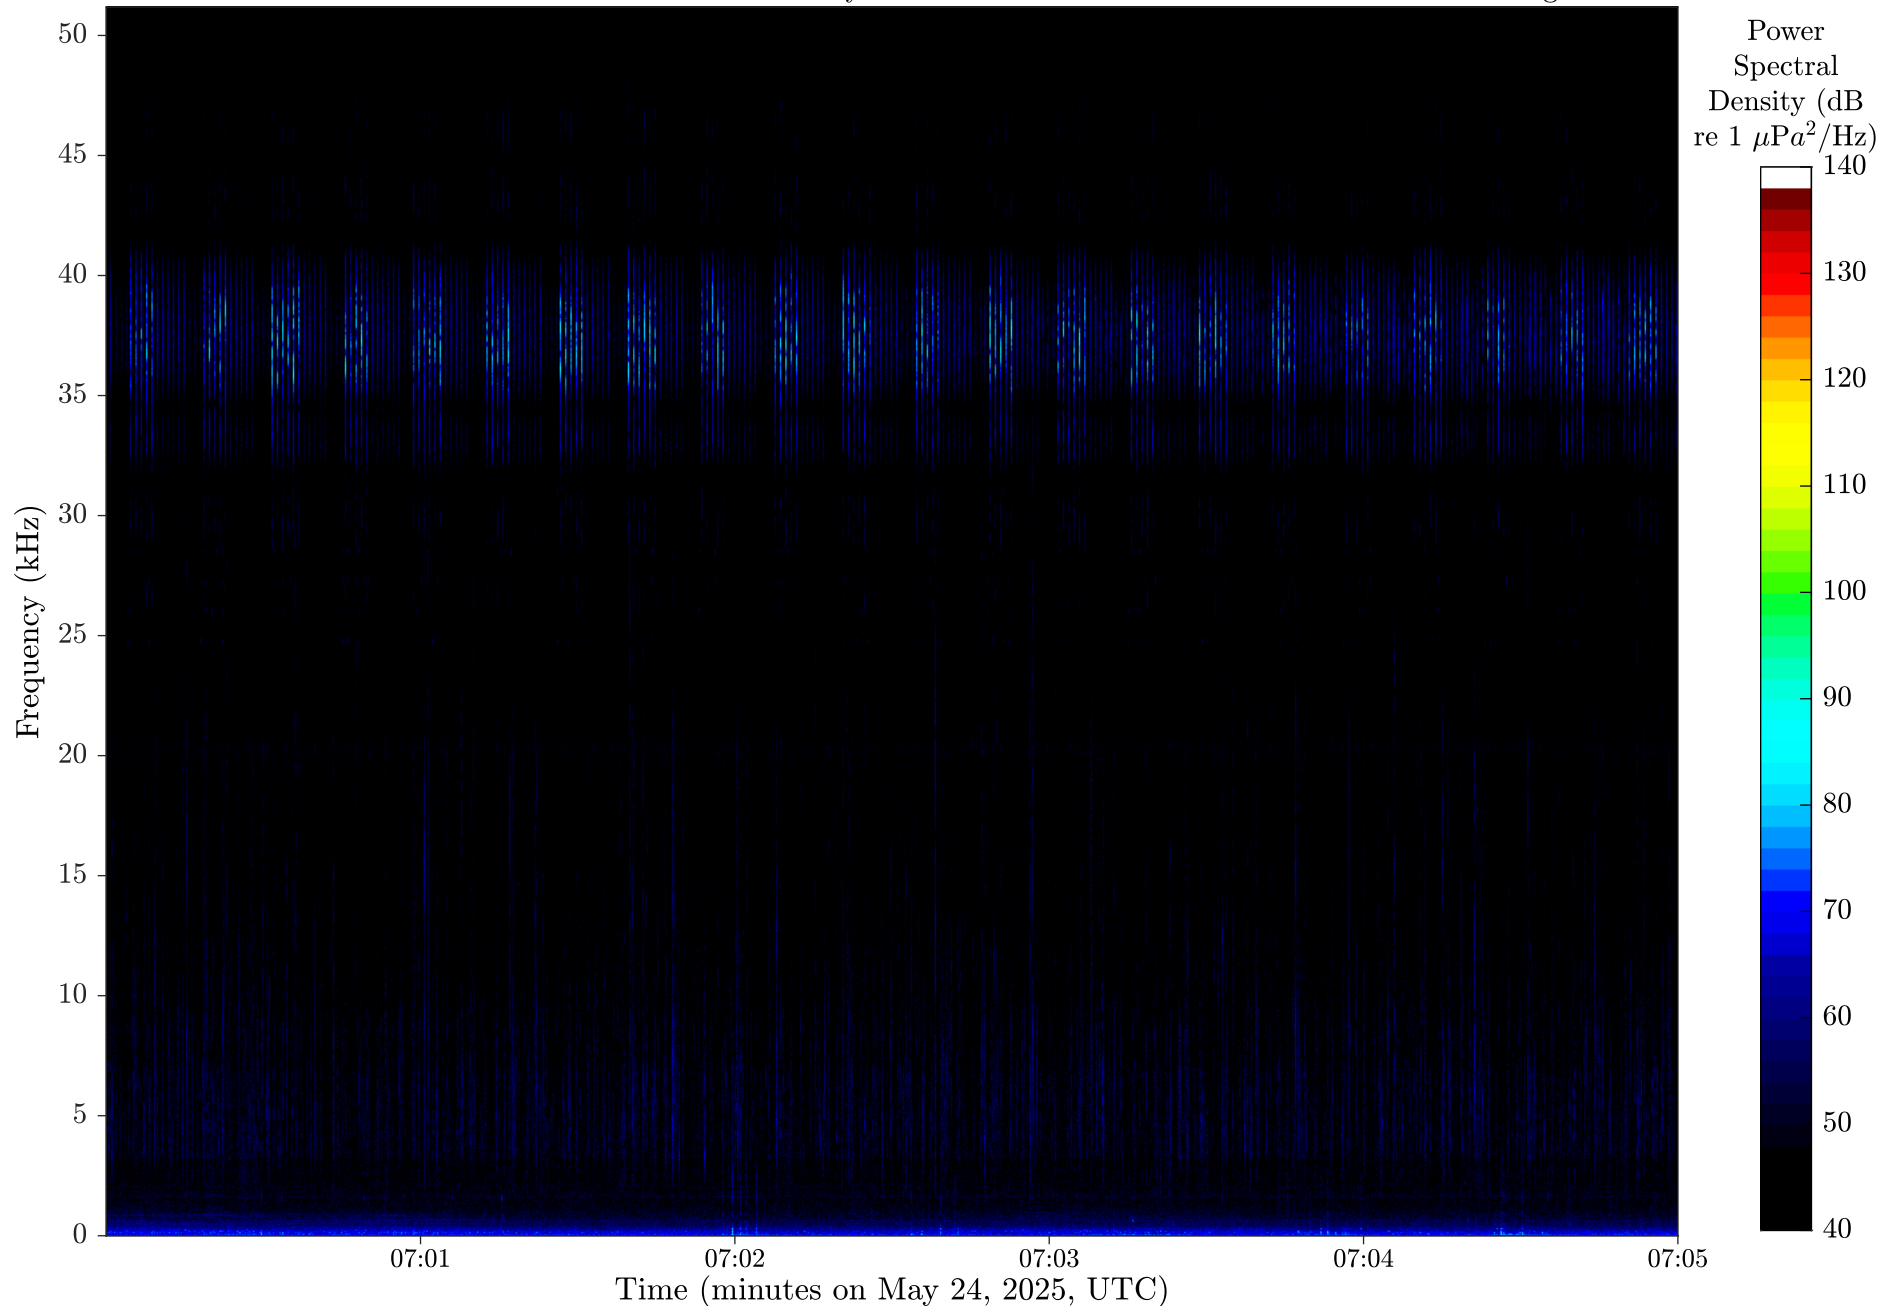


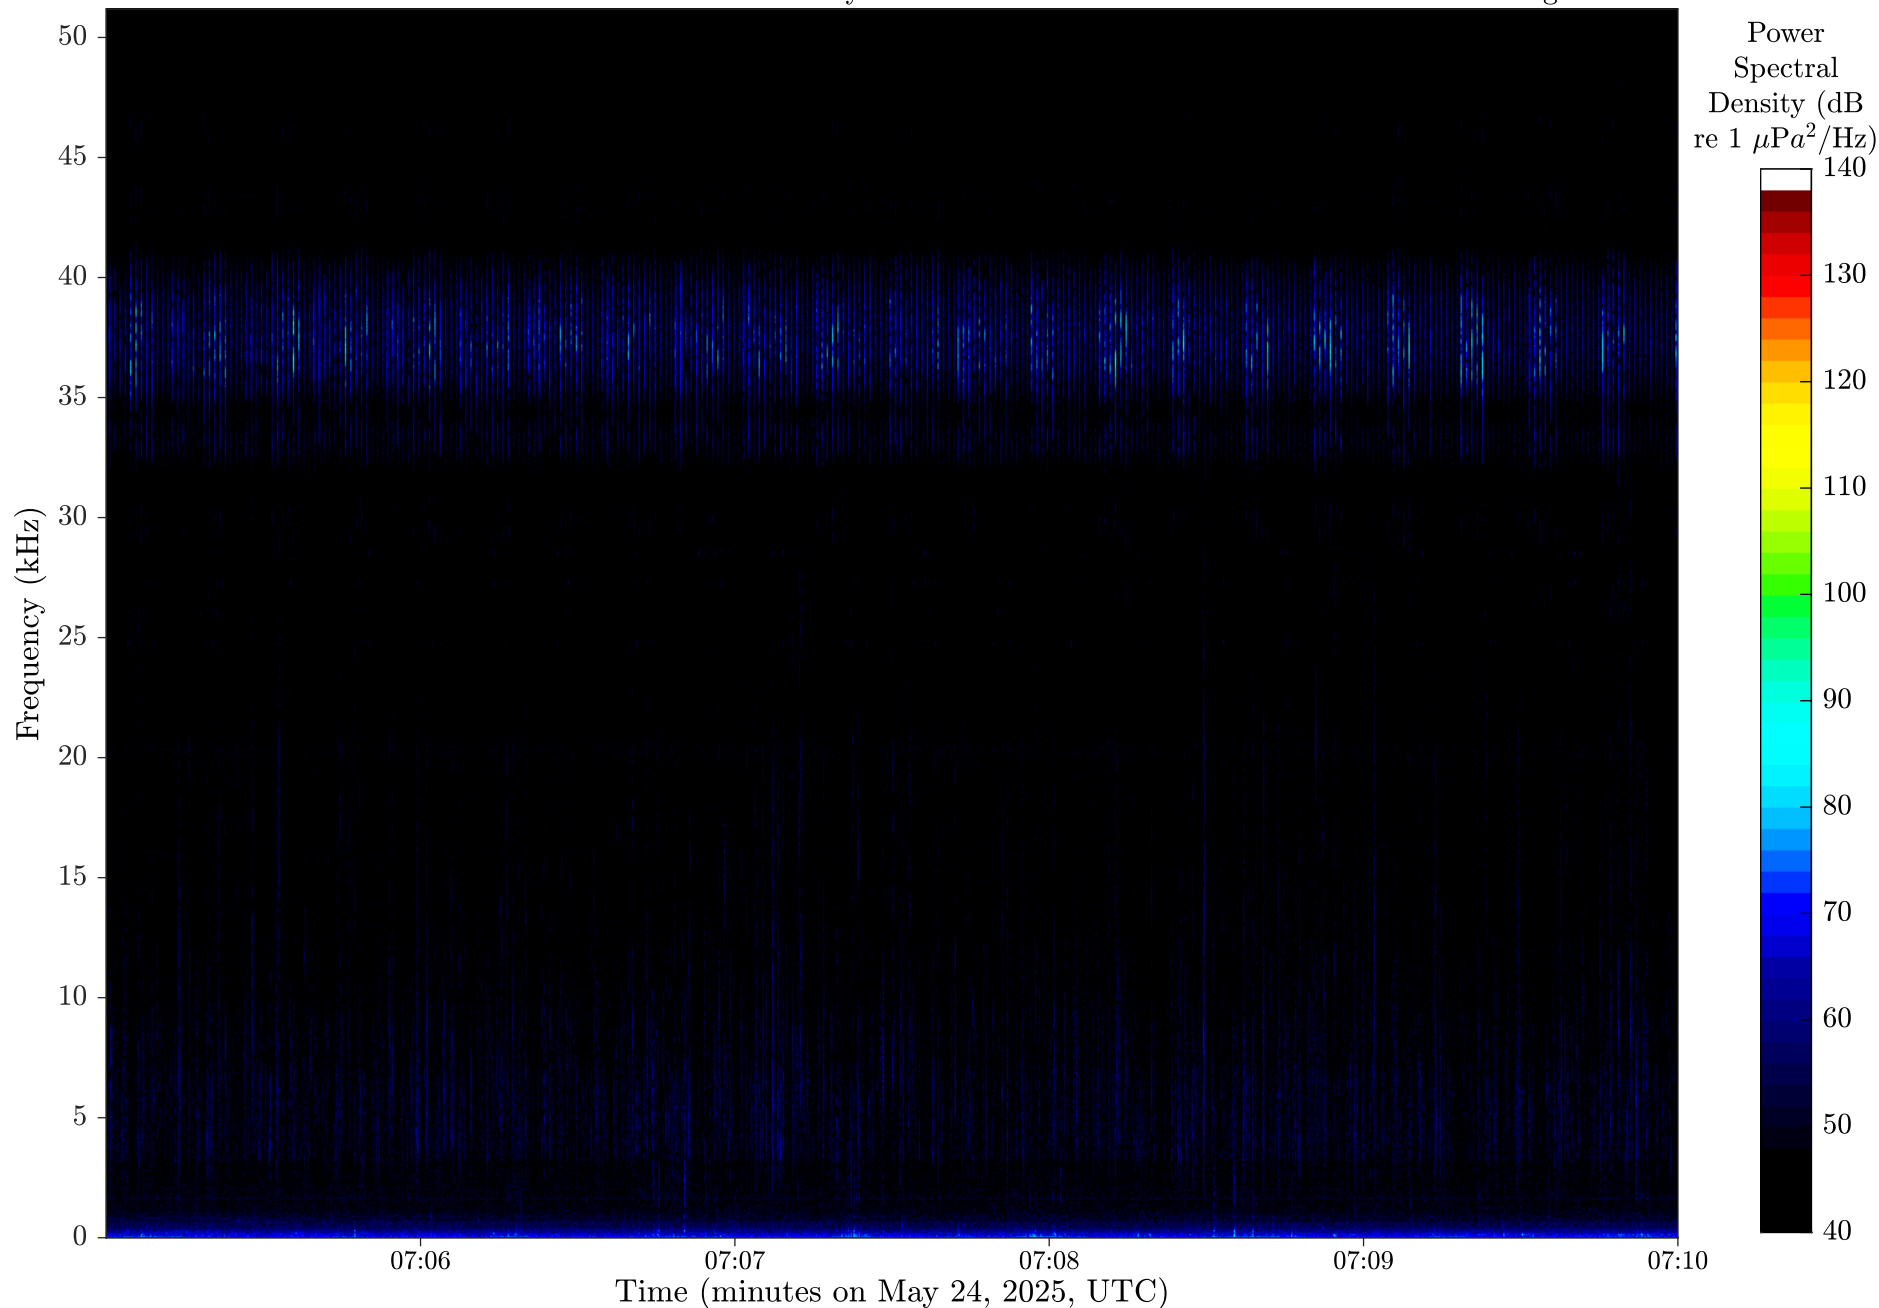

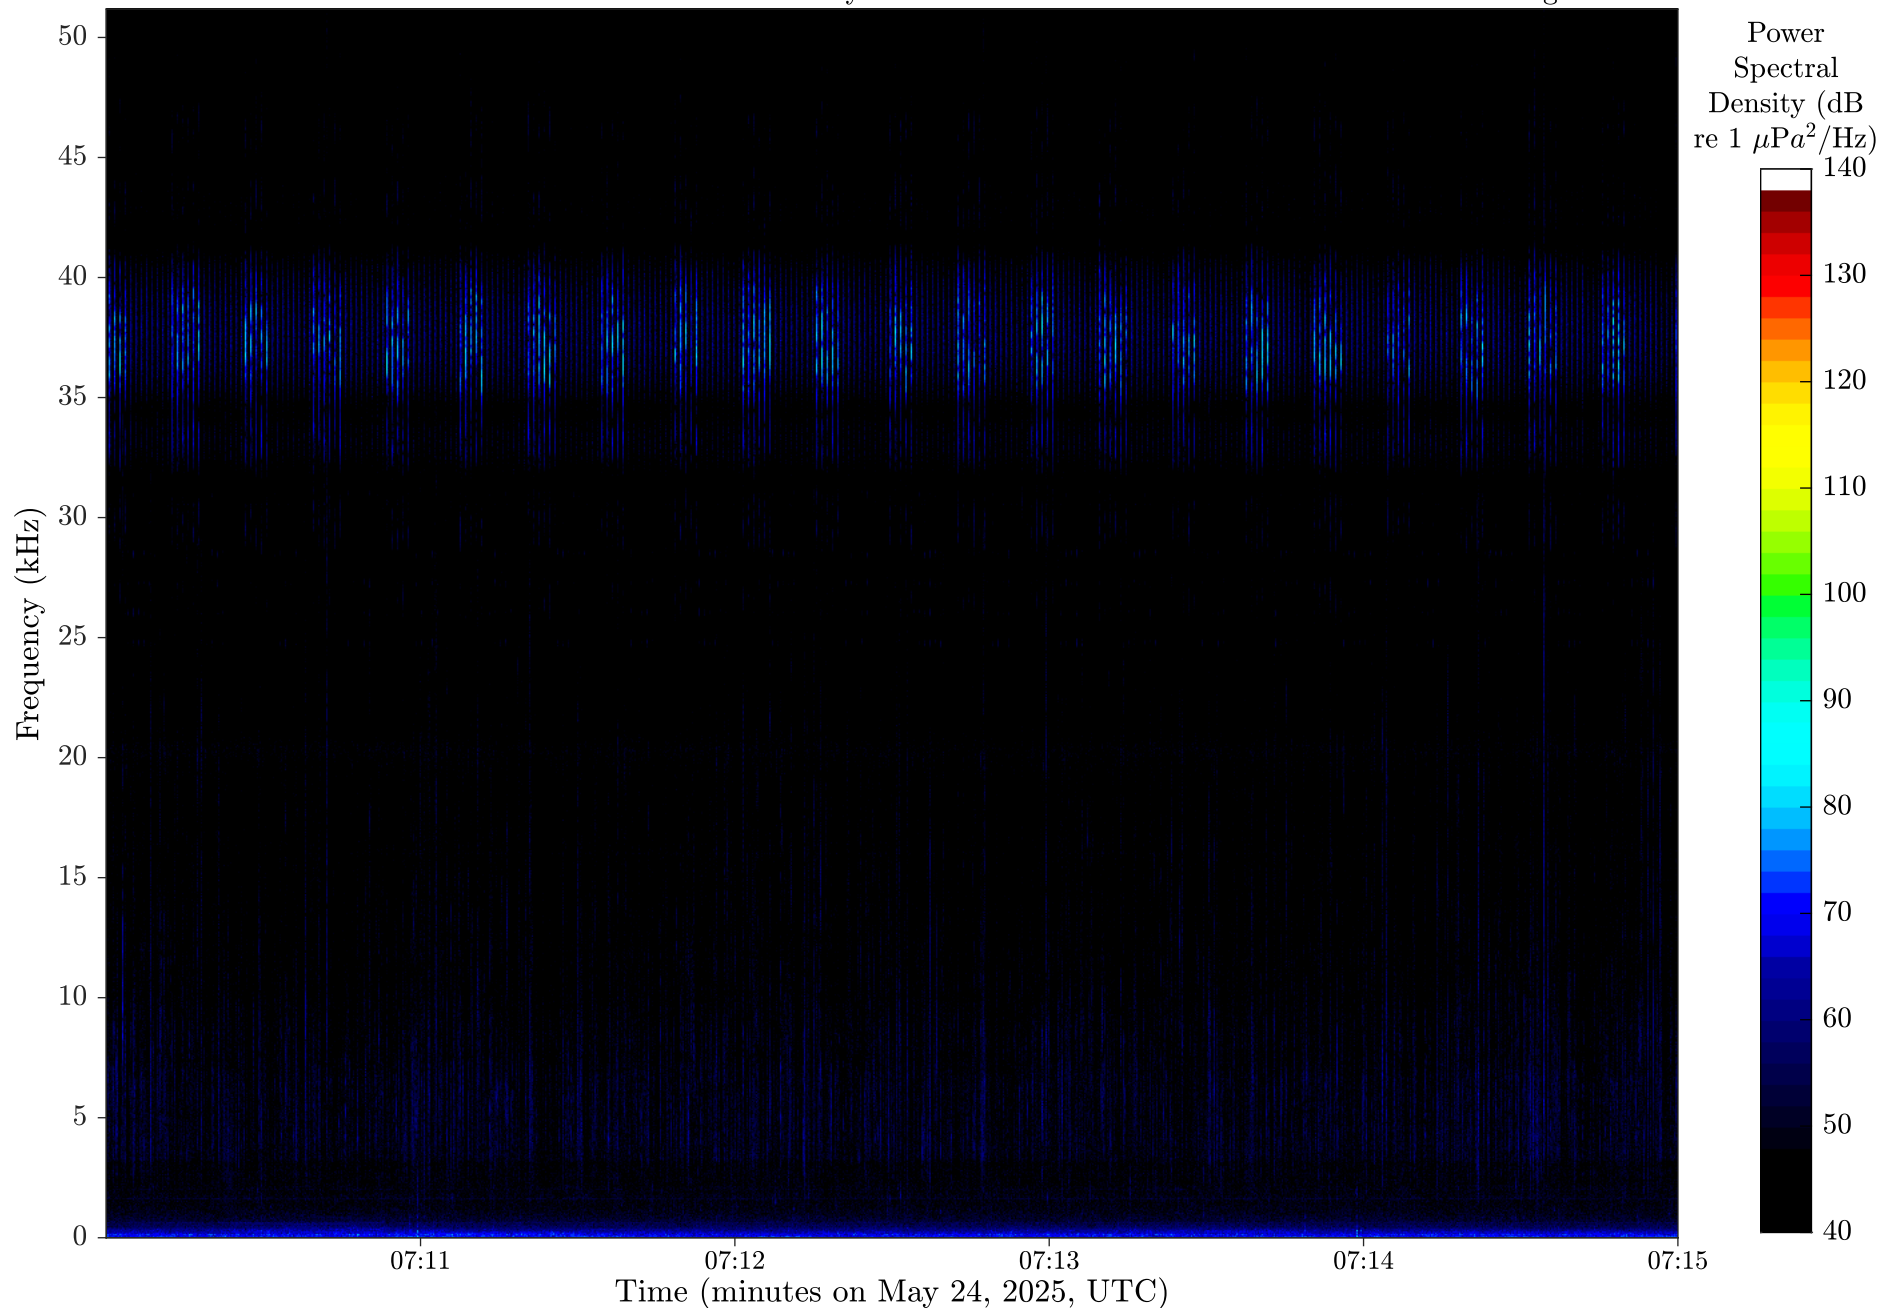


Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:22:39 UTC

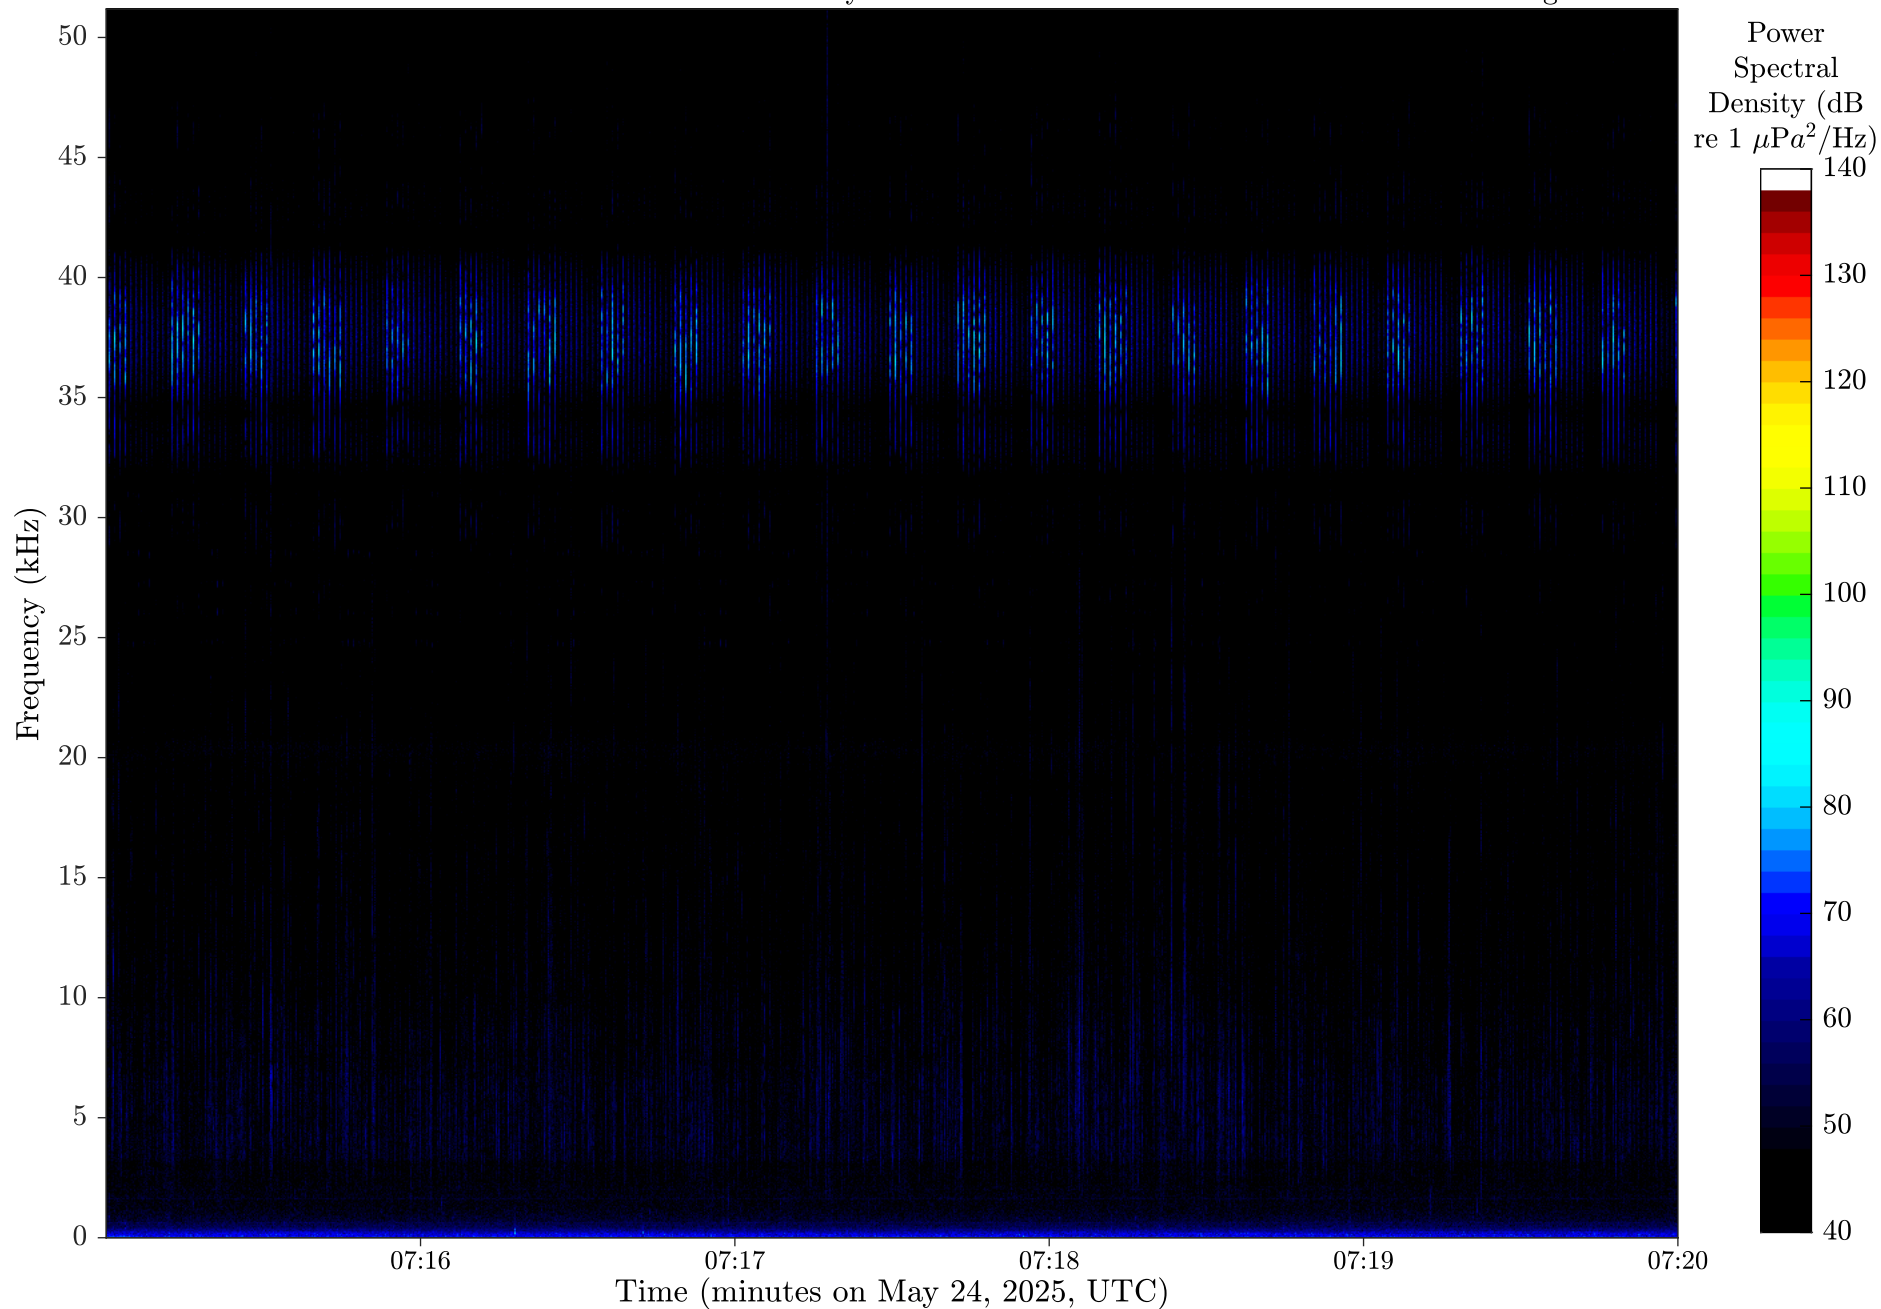

Comments: 36.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:22:46 UTC

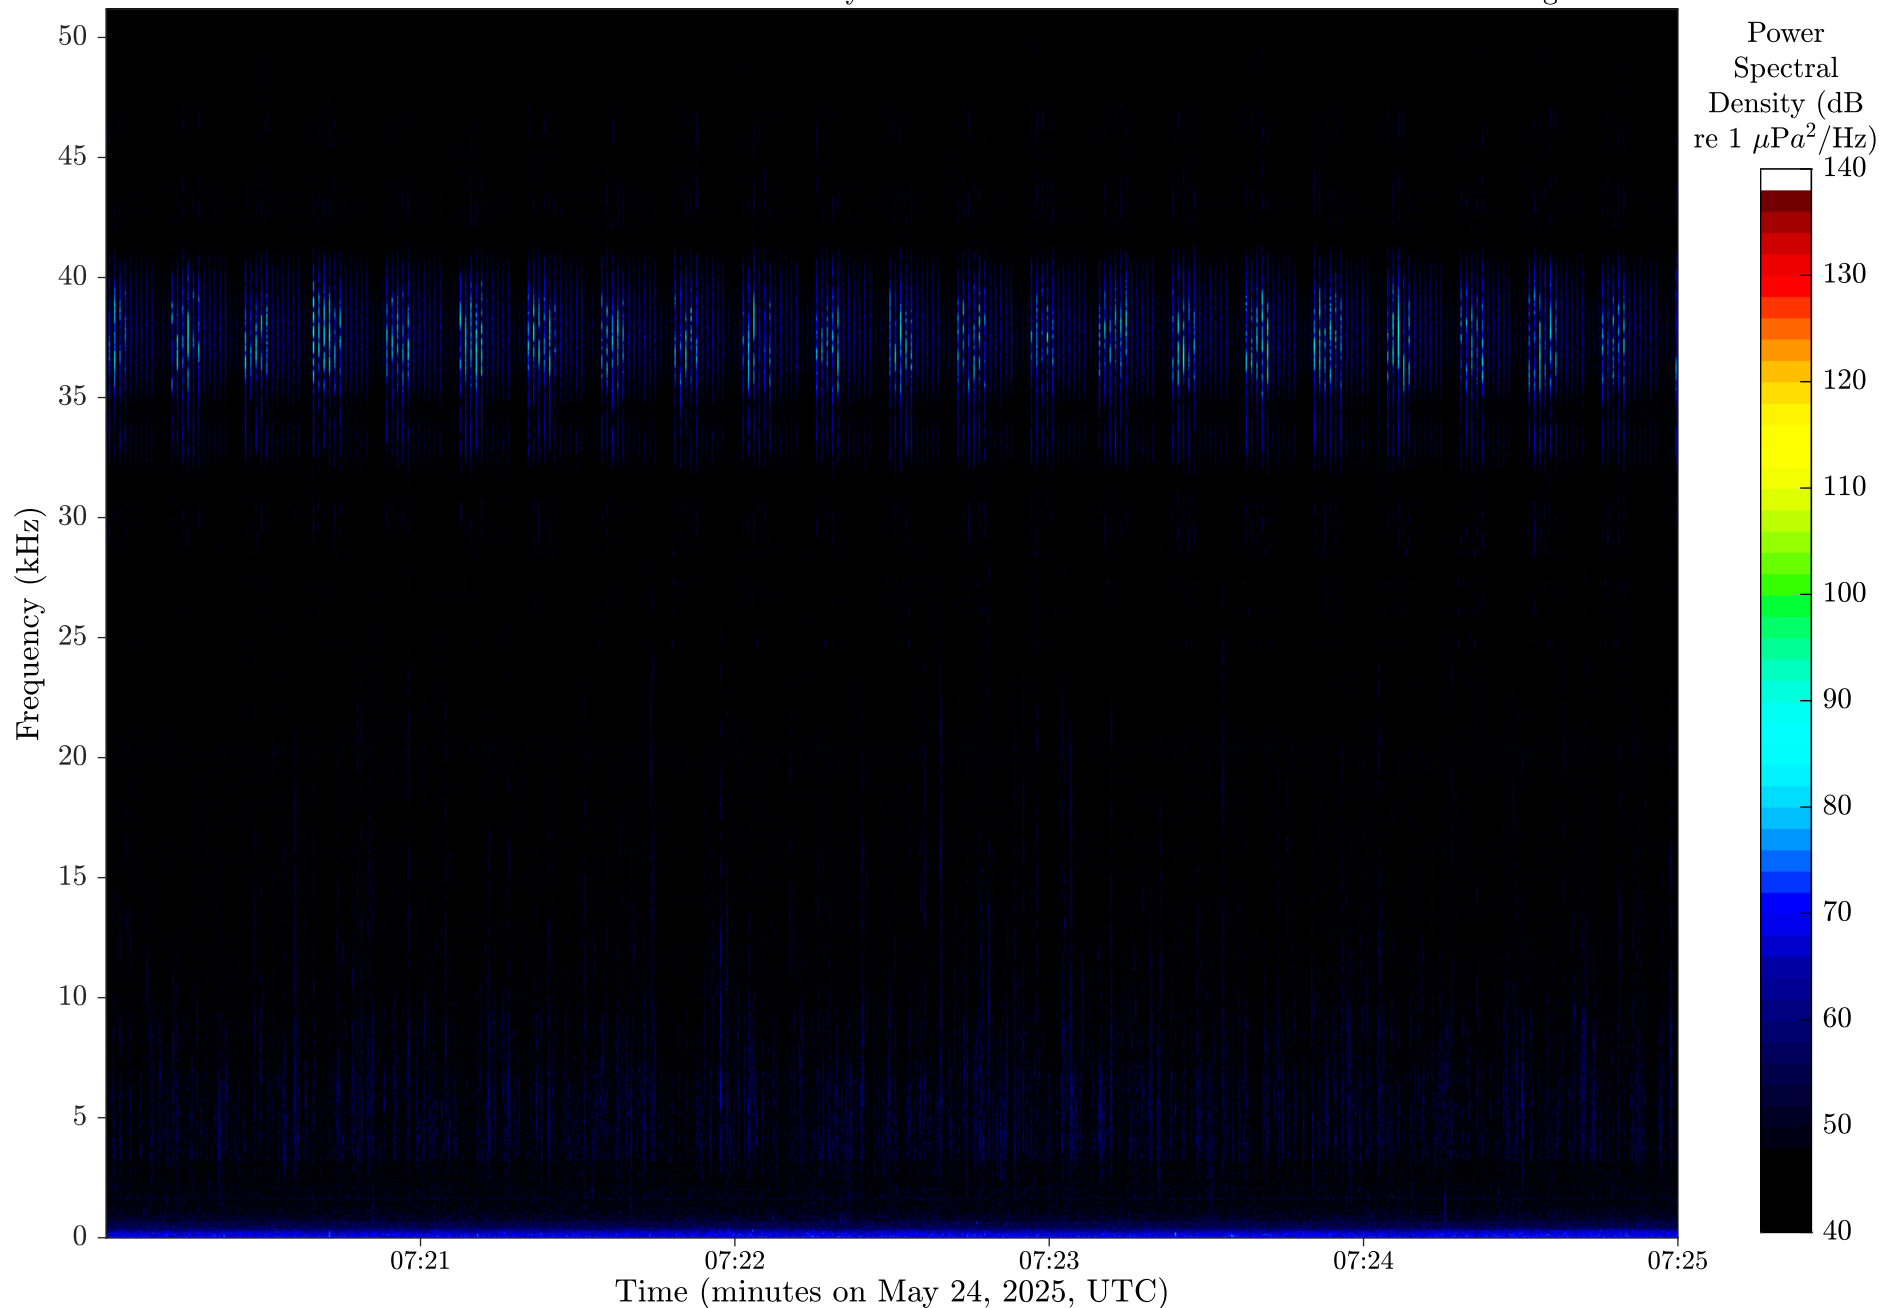

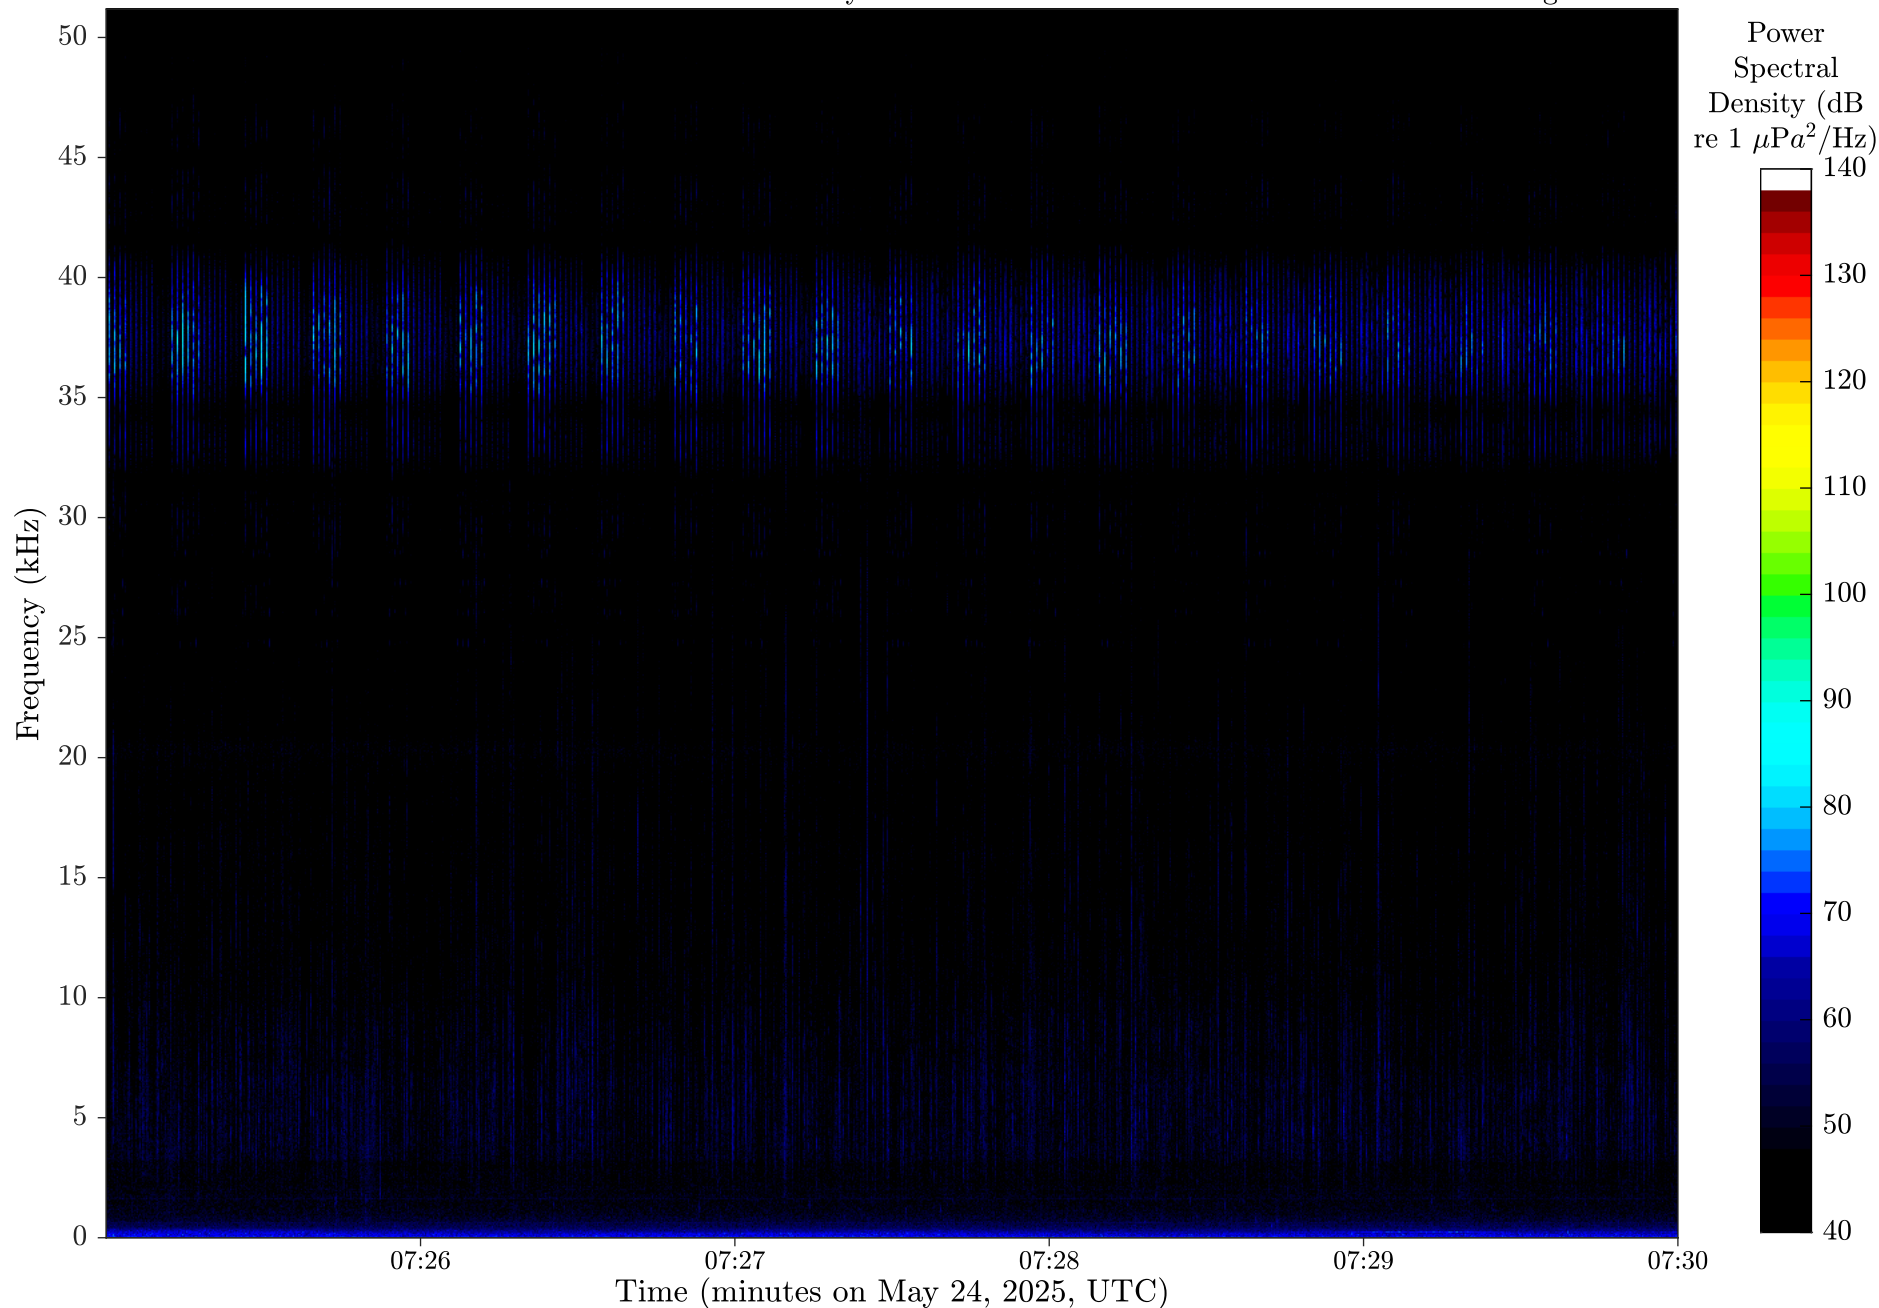


Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:01 UTC

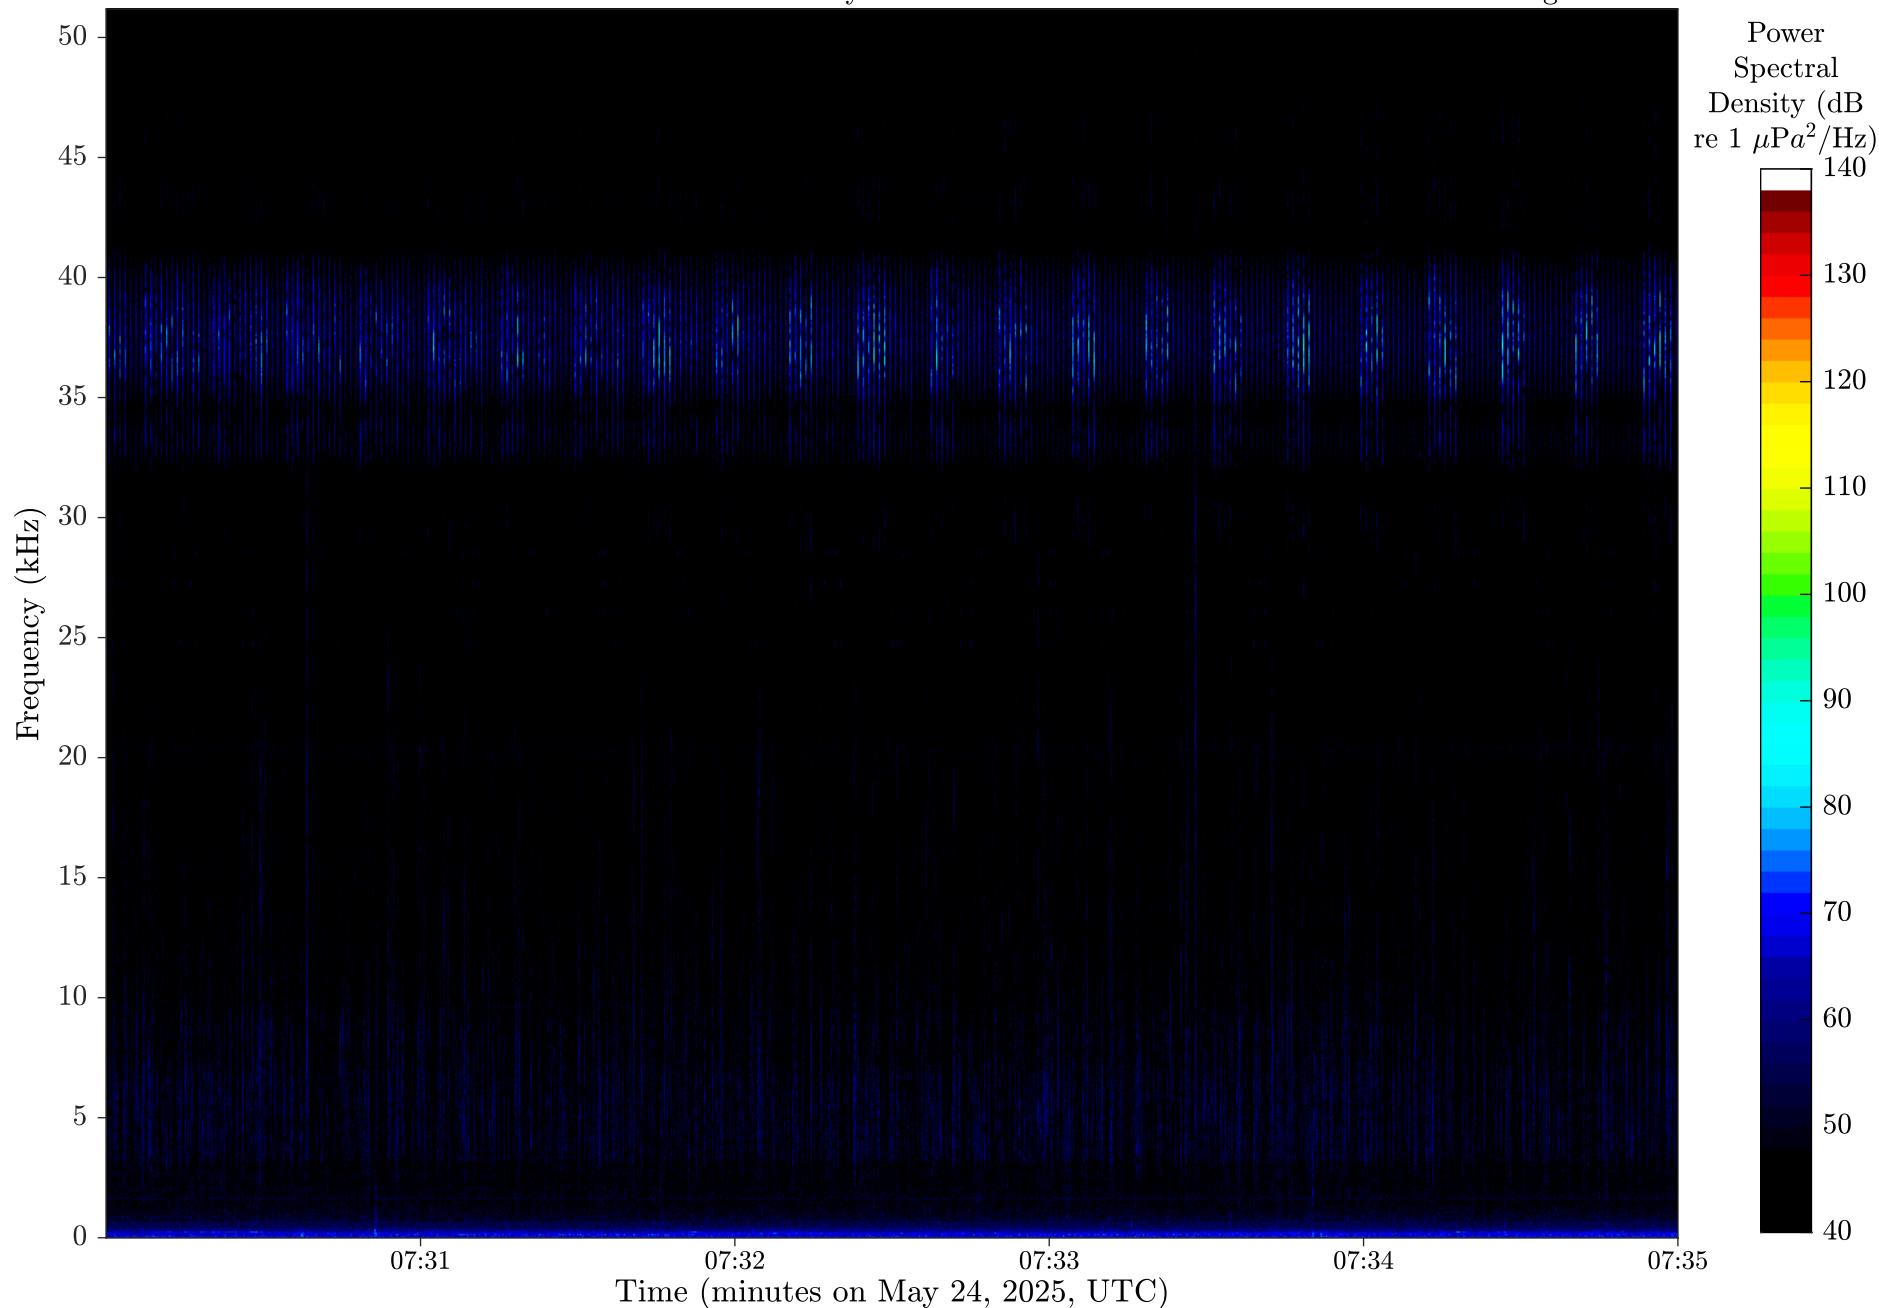


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:08 UTC

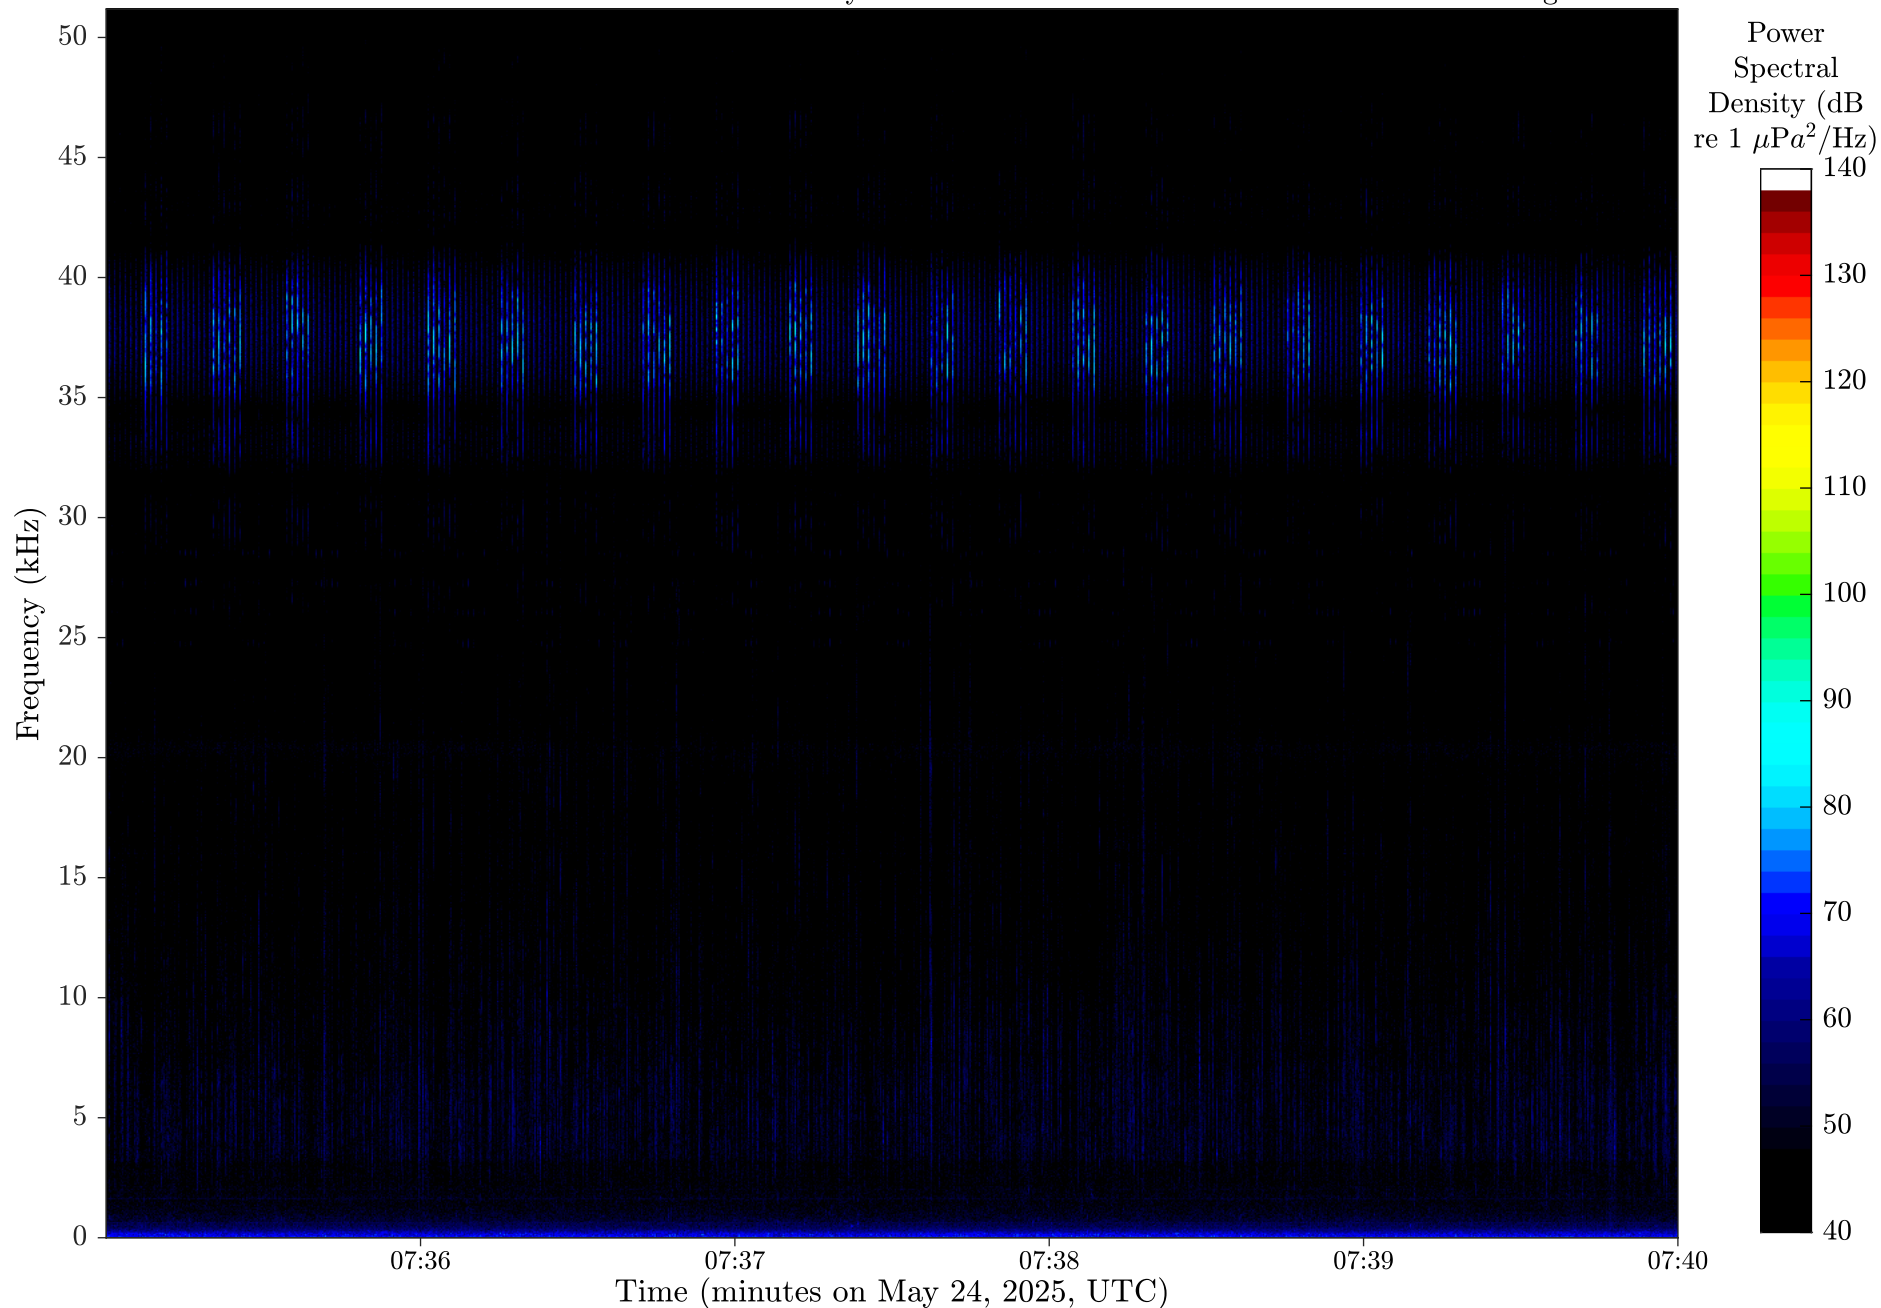


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:14 UTC

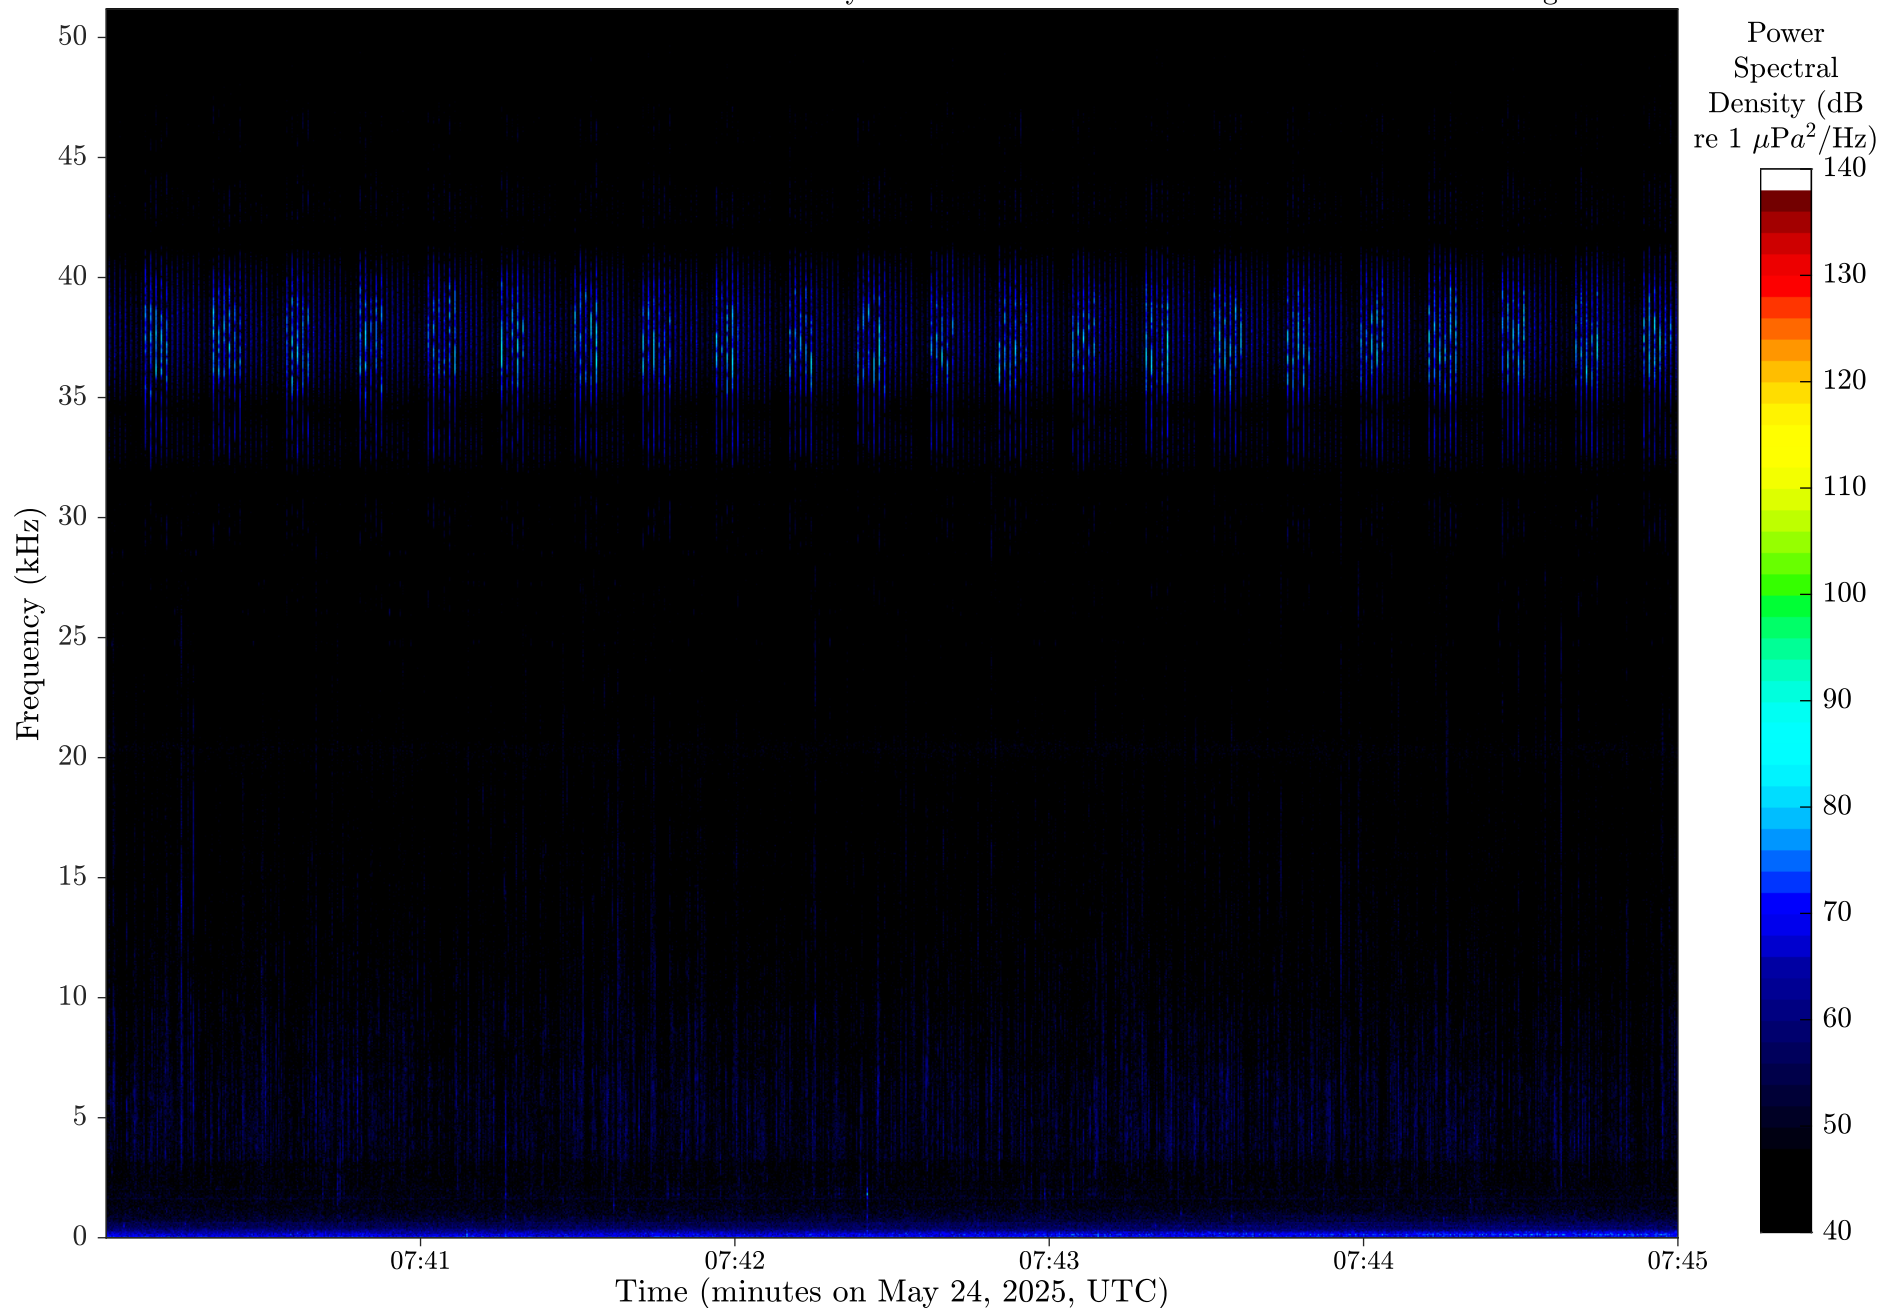


Comments: 36.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:22 UTC

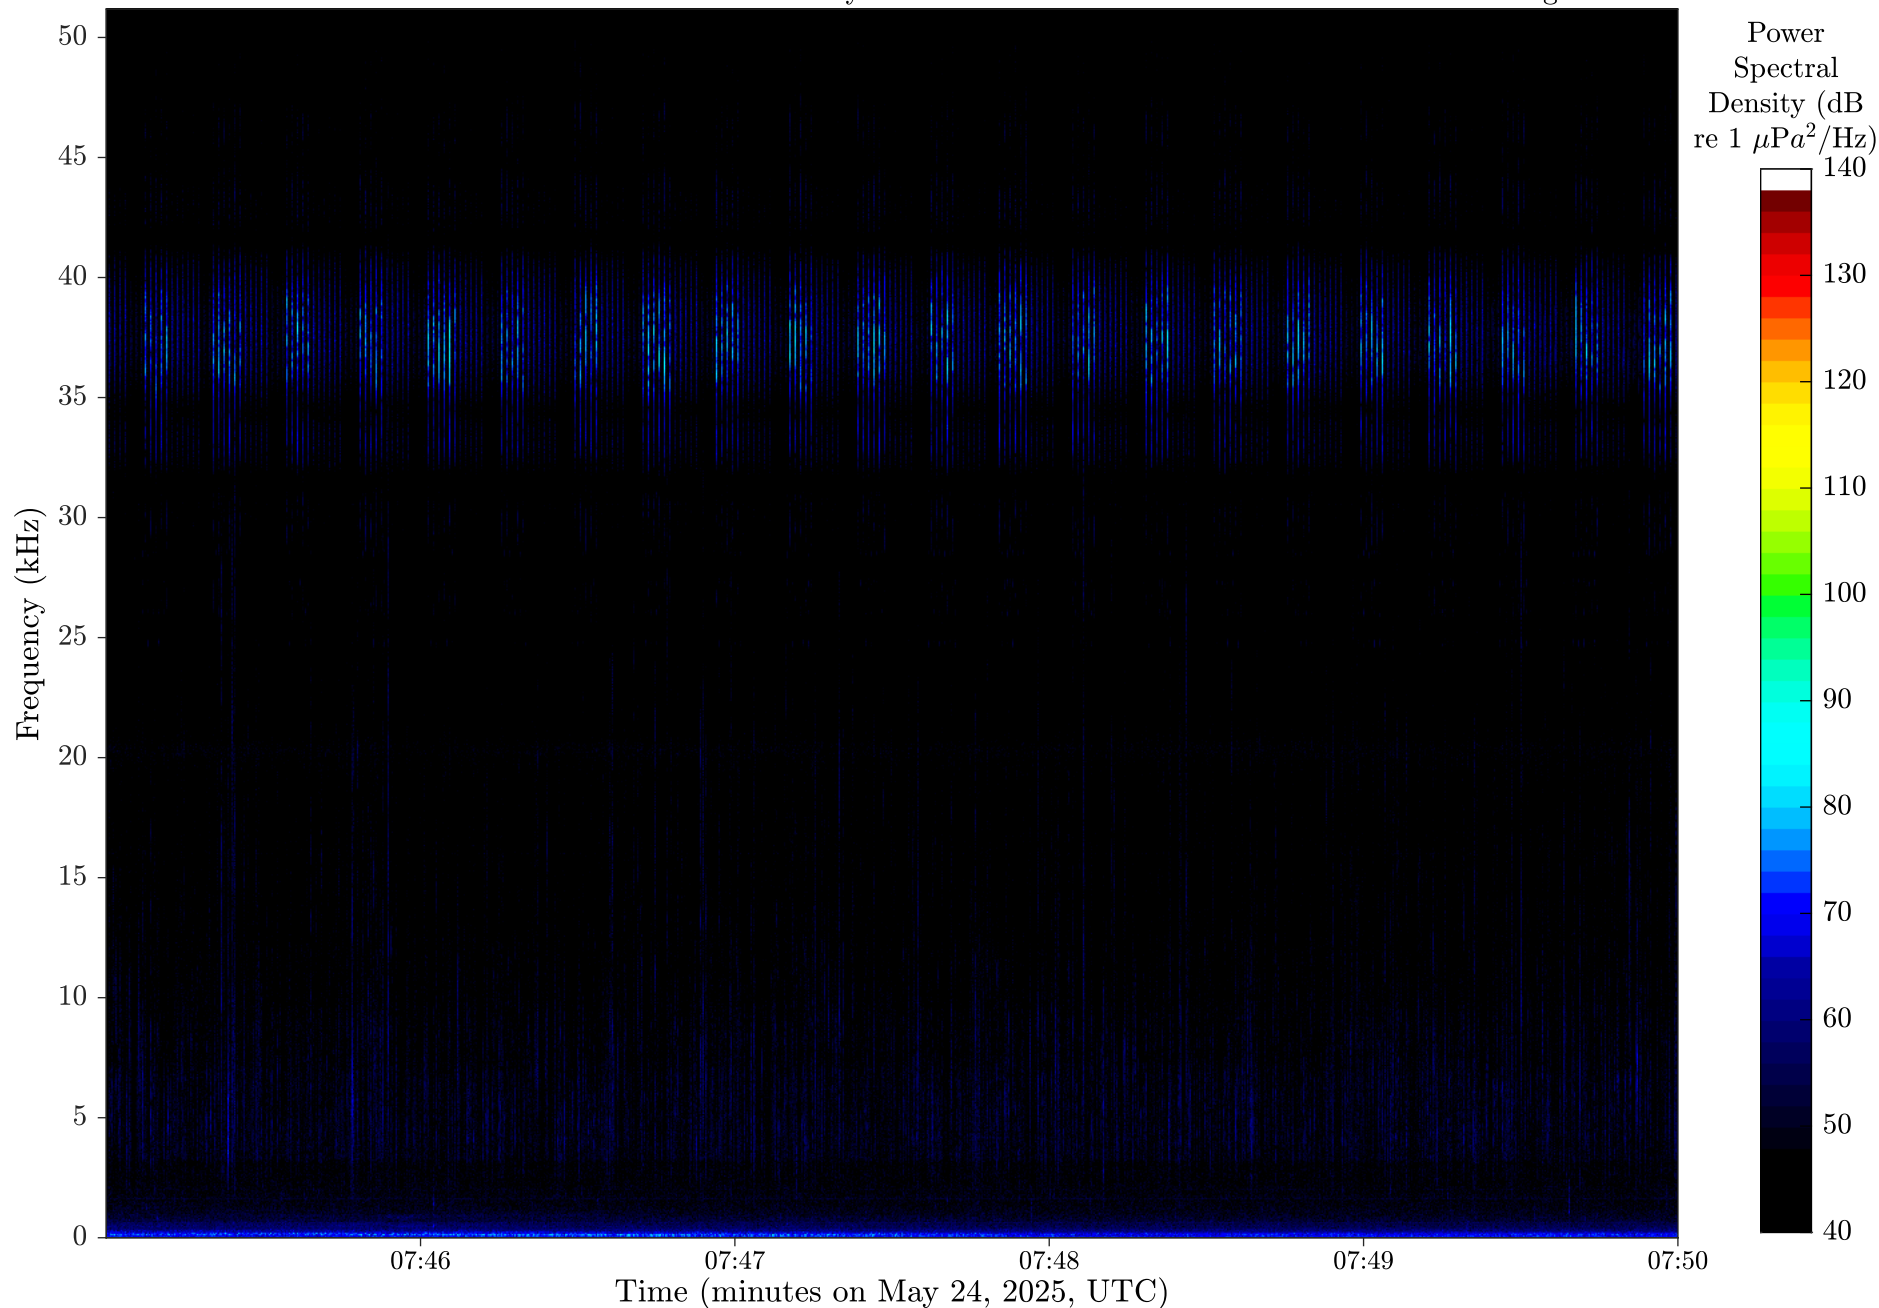


Comments: 36.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:29 UTC

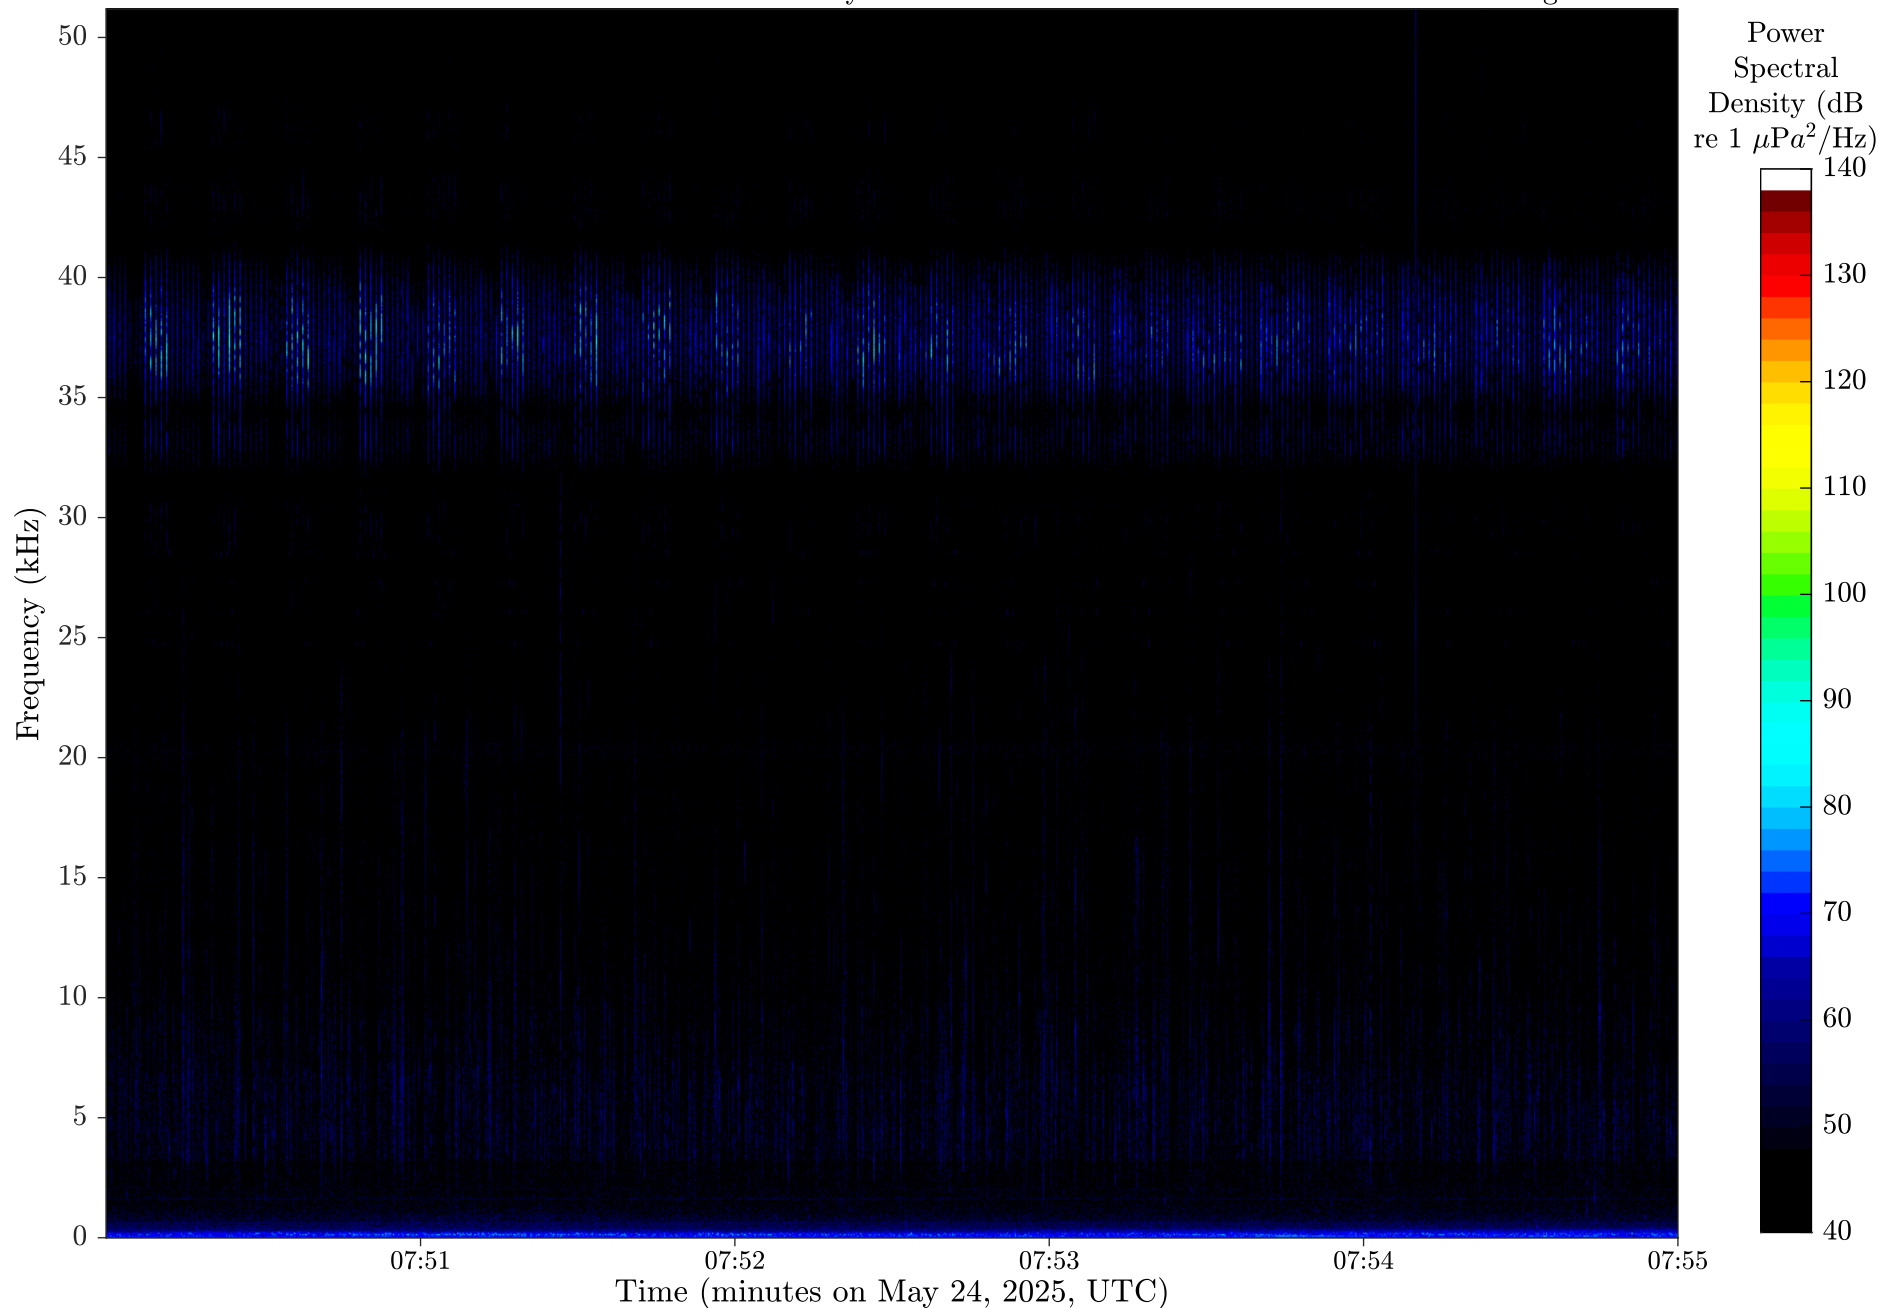


Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:36 UTC

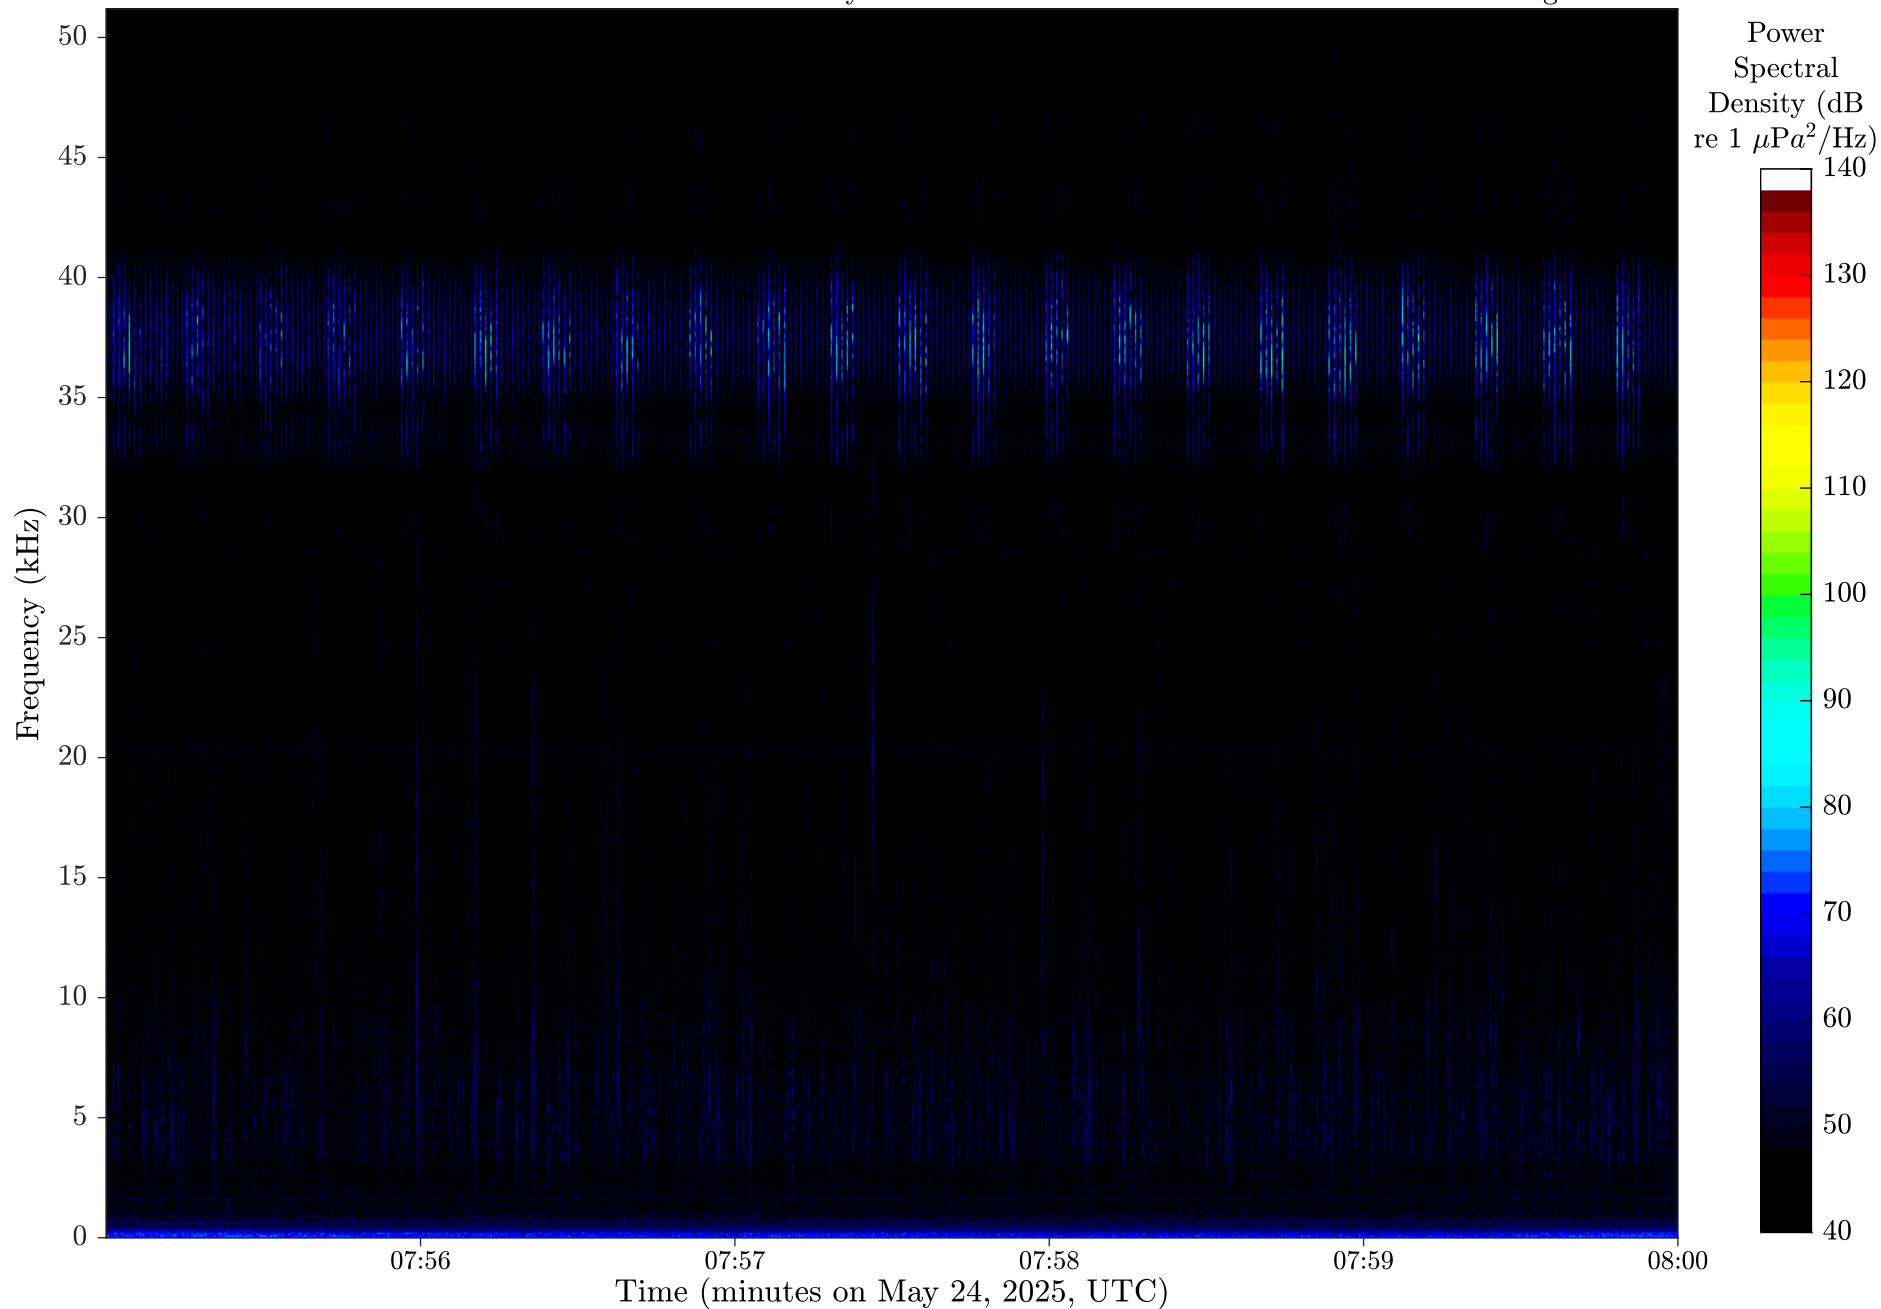


Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:43 UTC

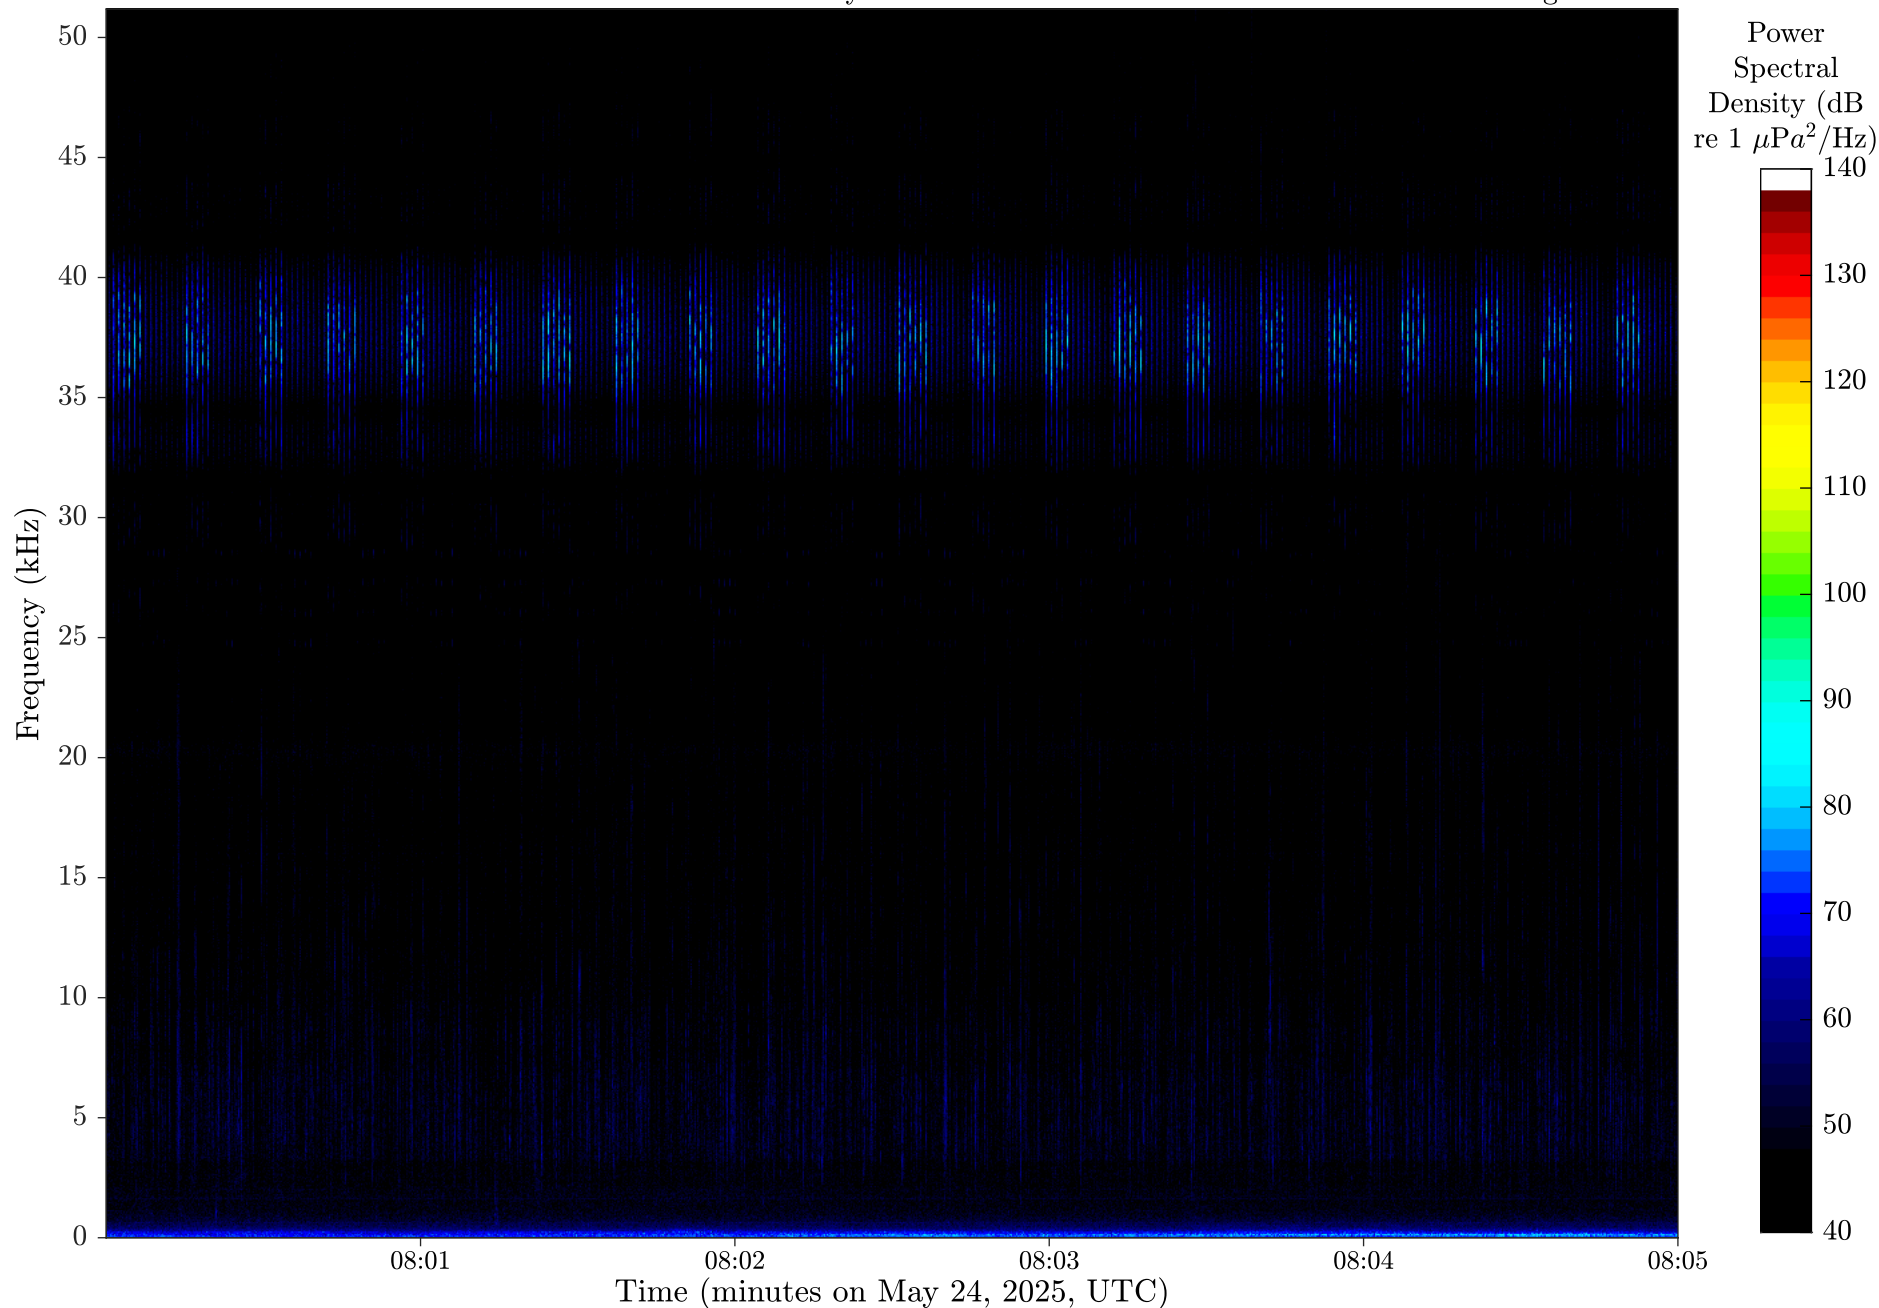


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:50 UTC

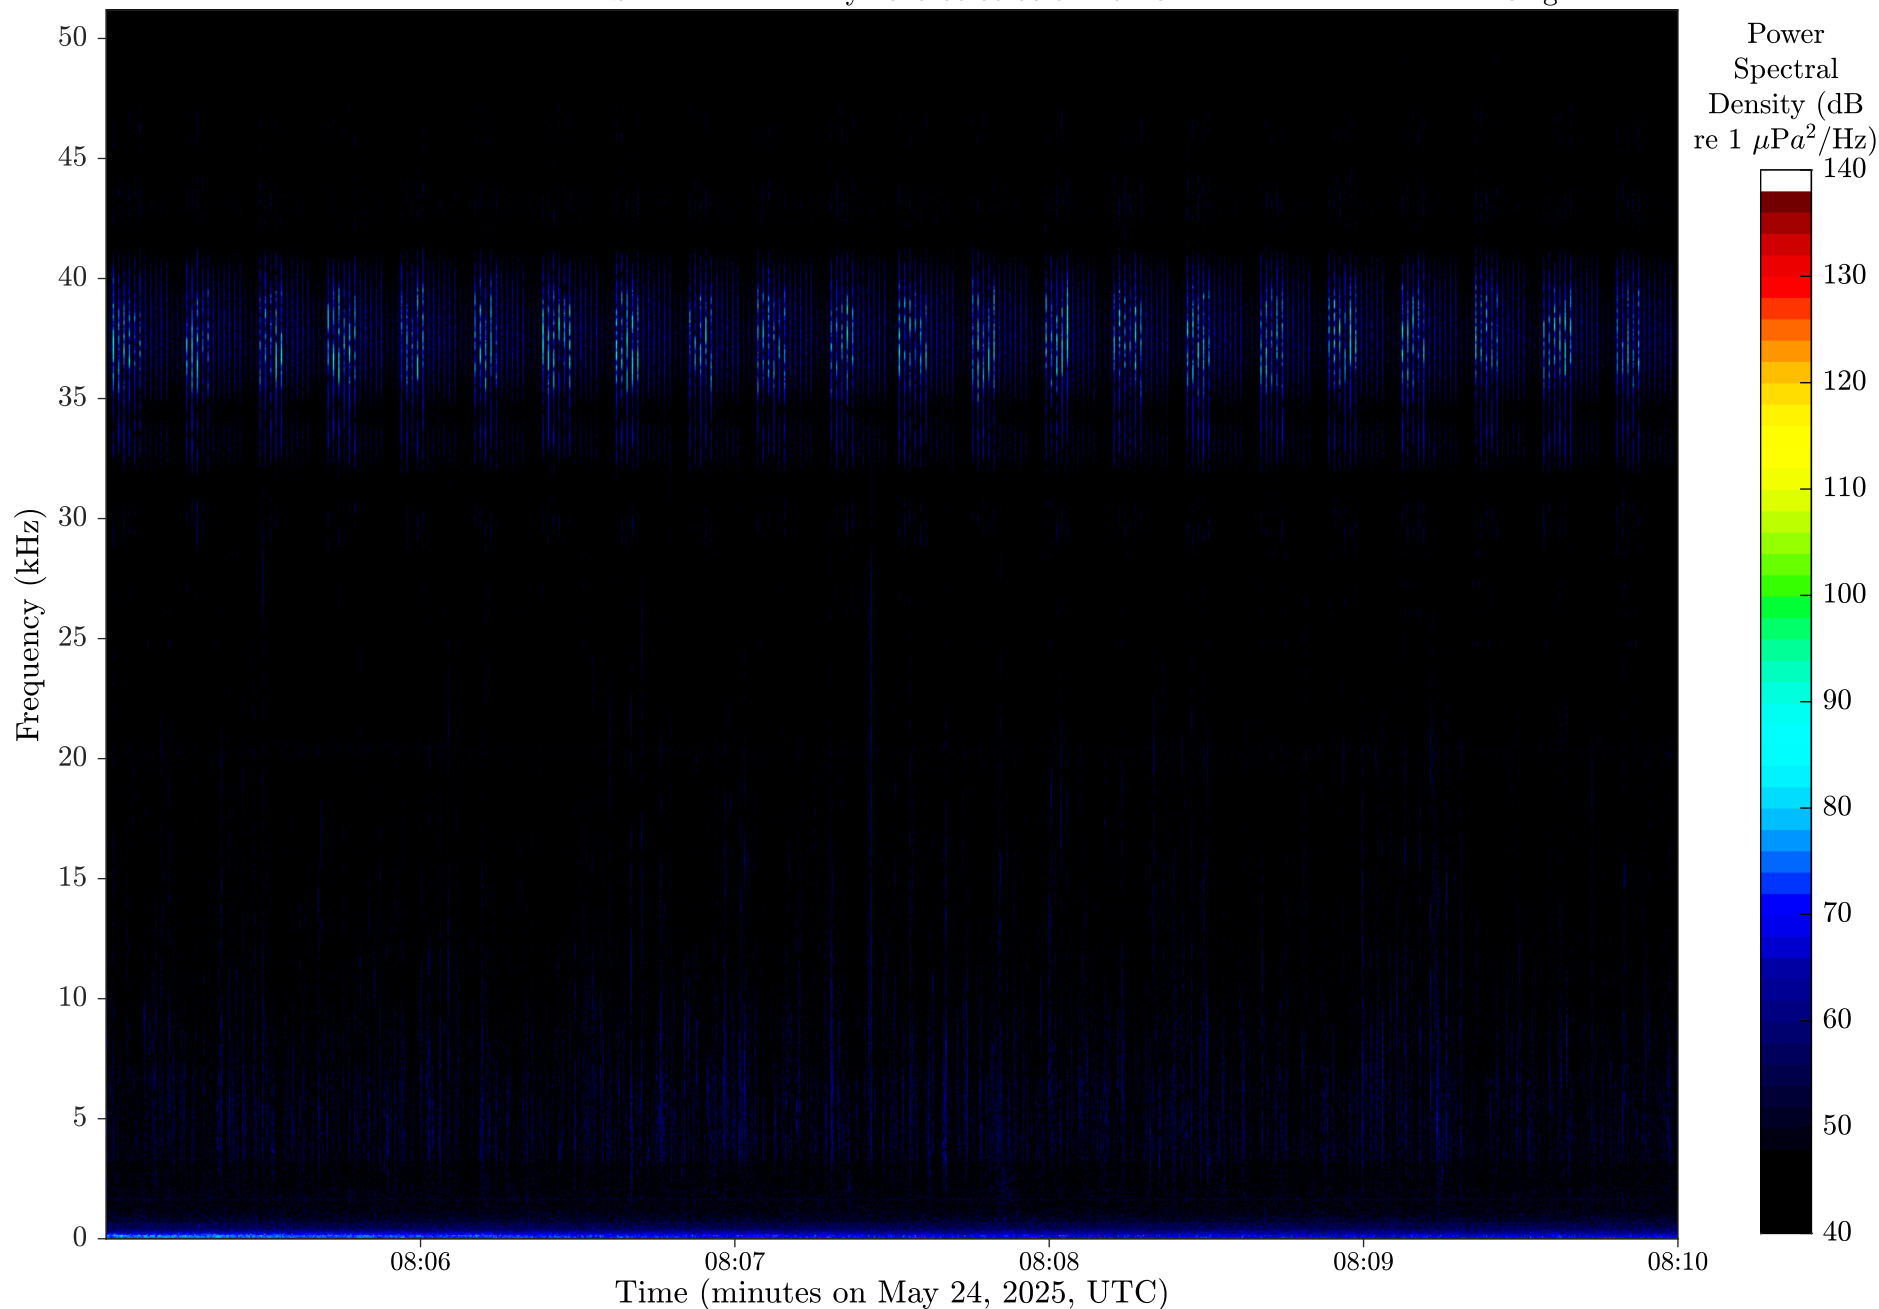


Comments: 36.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:58 UTC

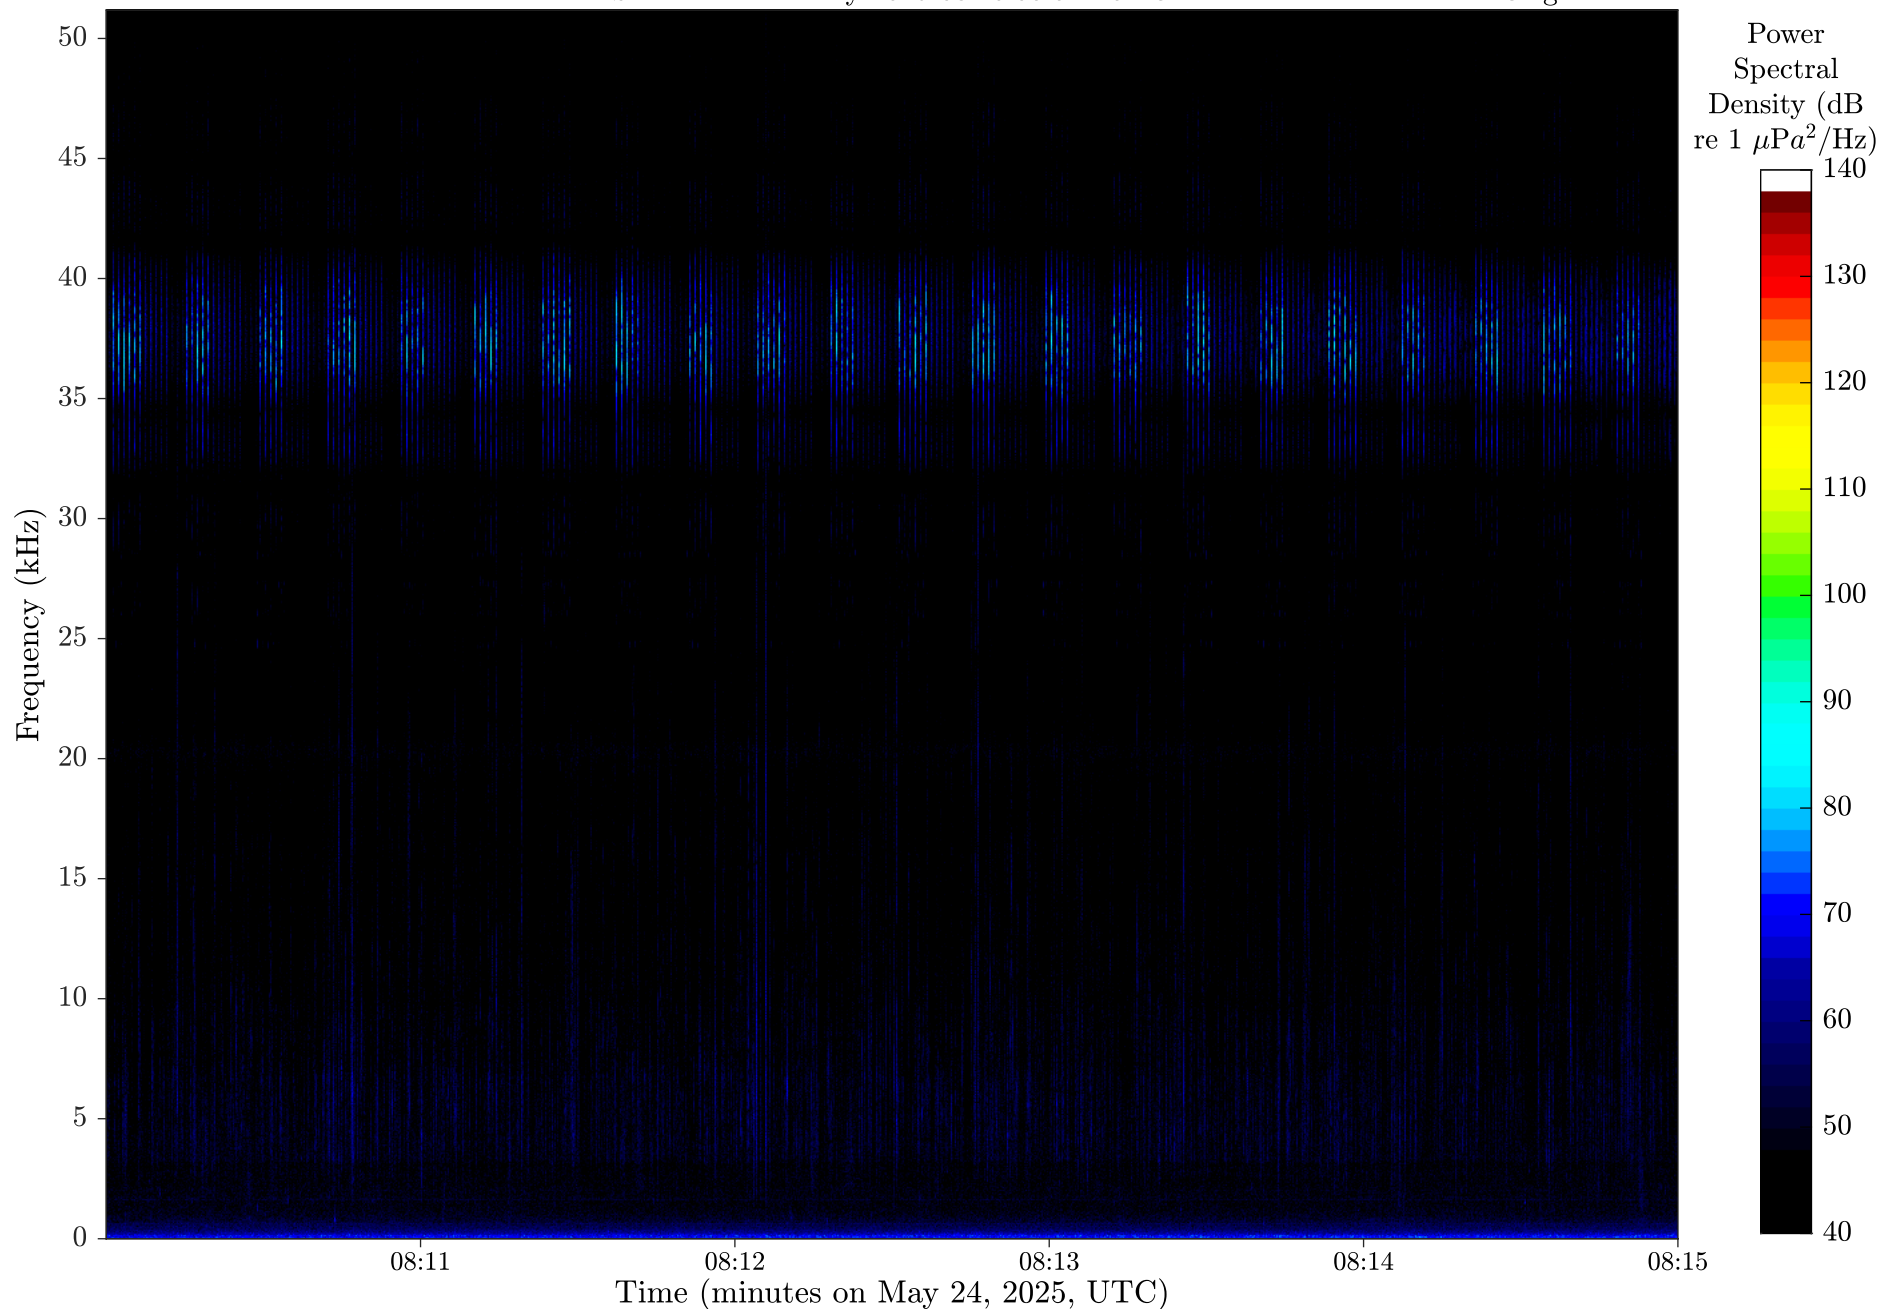


Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:24:05 UTC

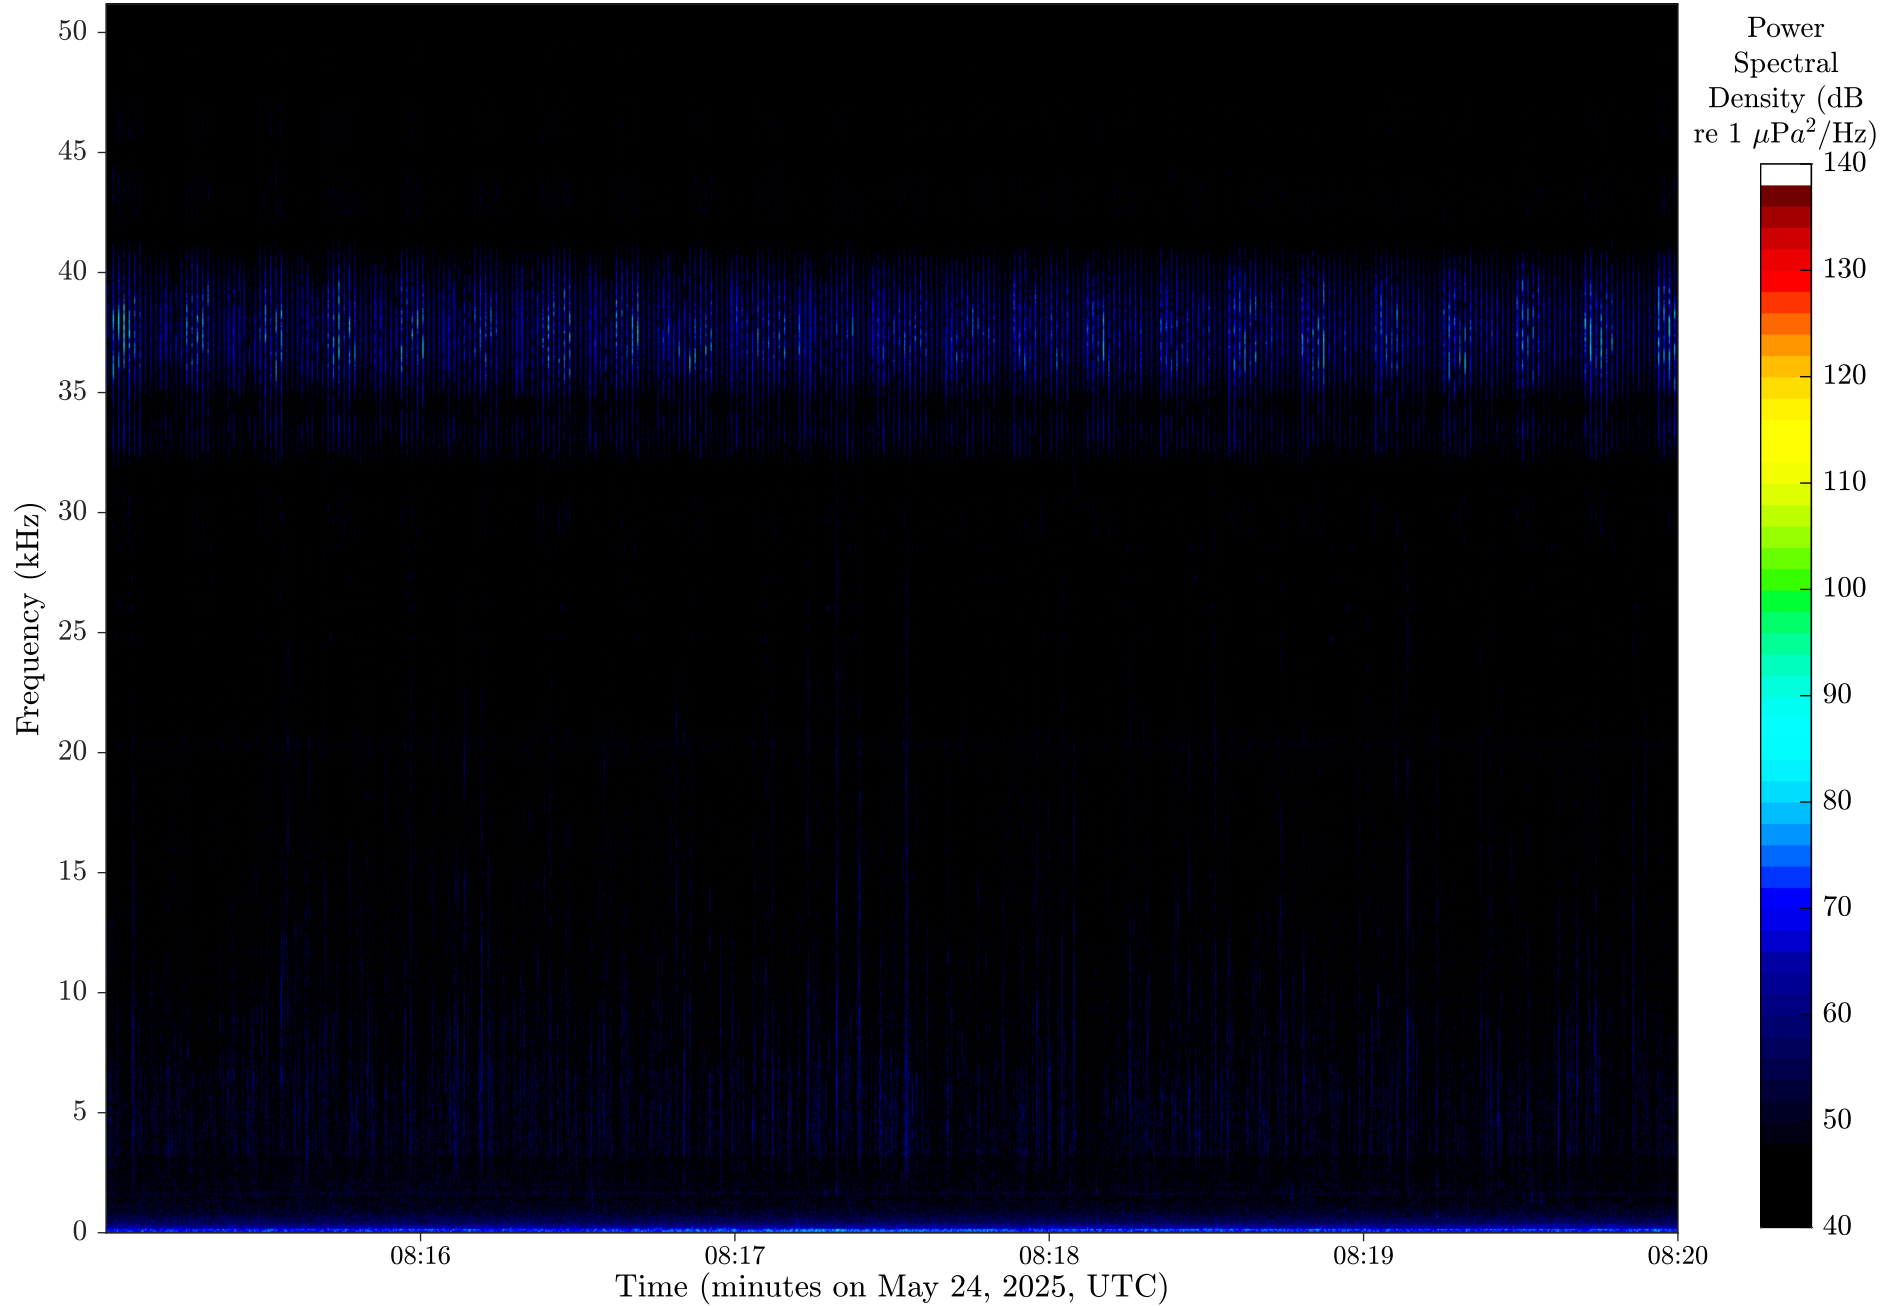


Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:24:12 UTC

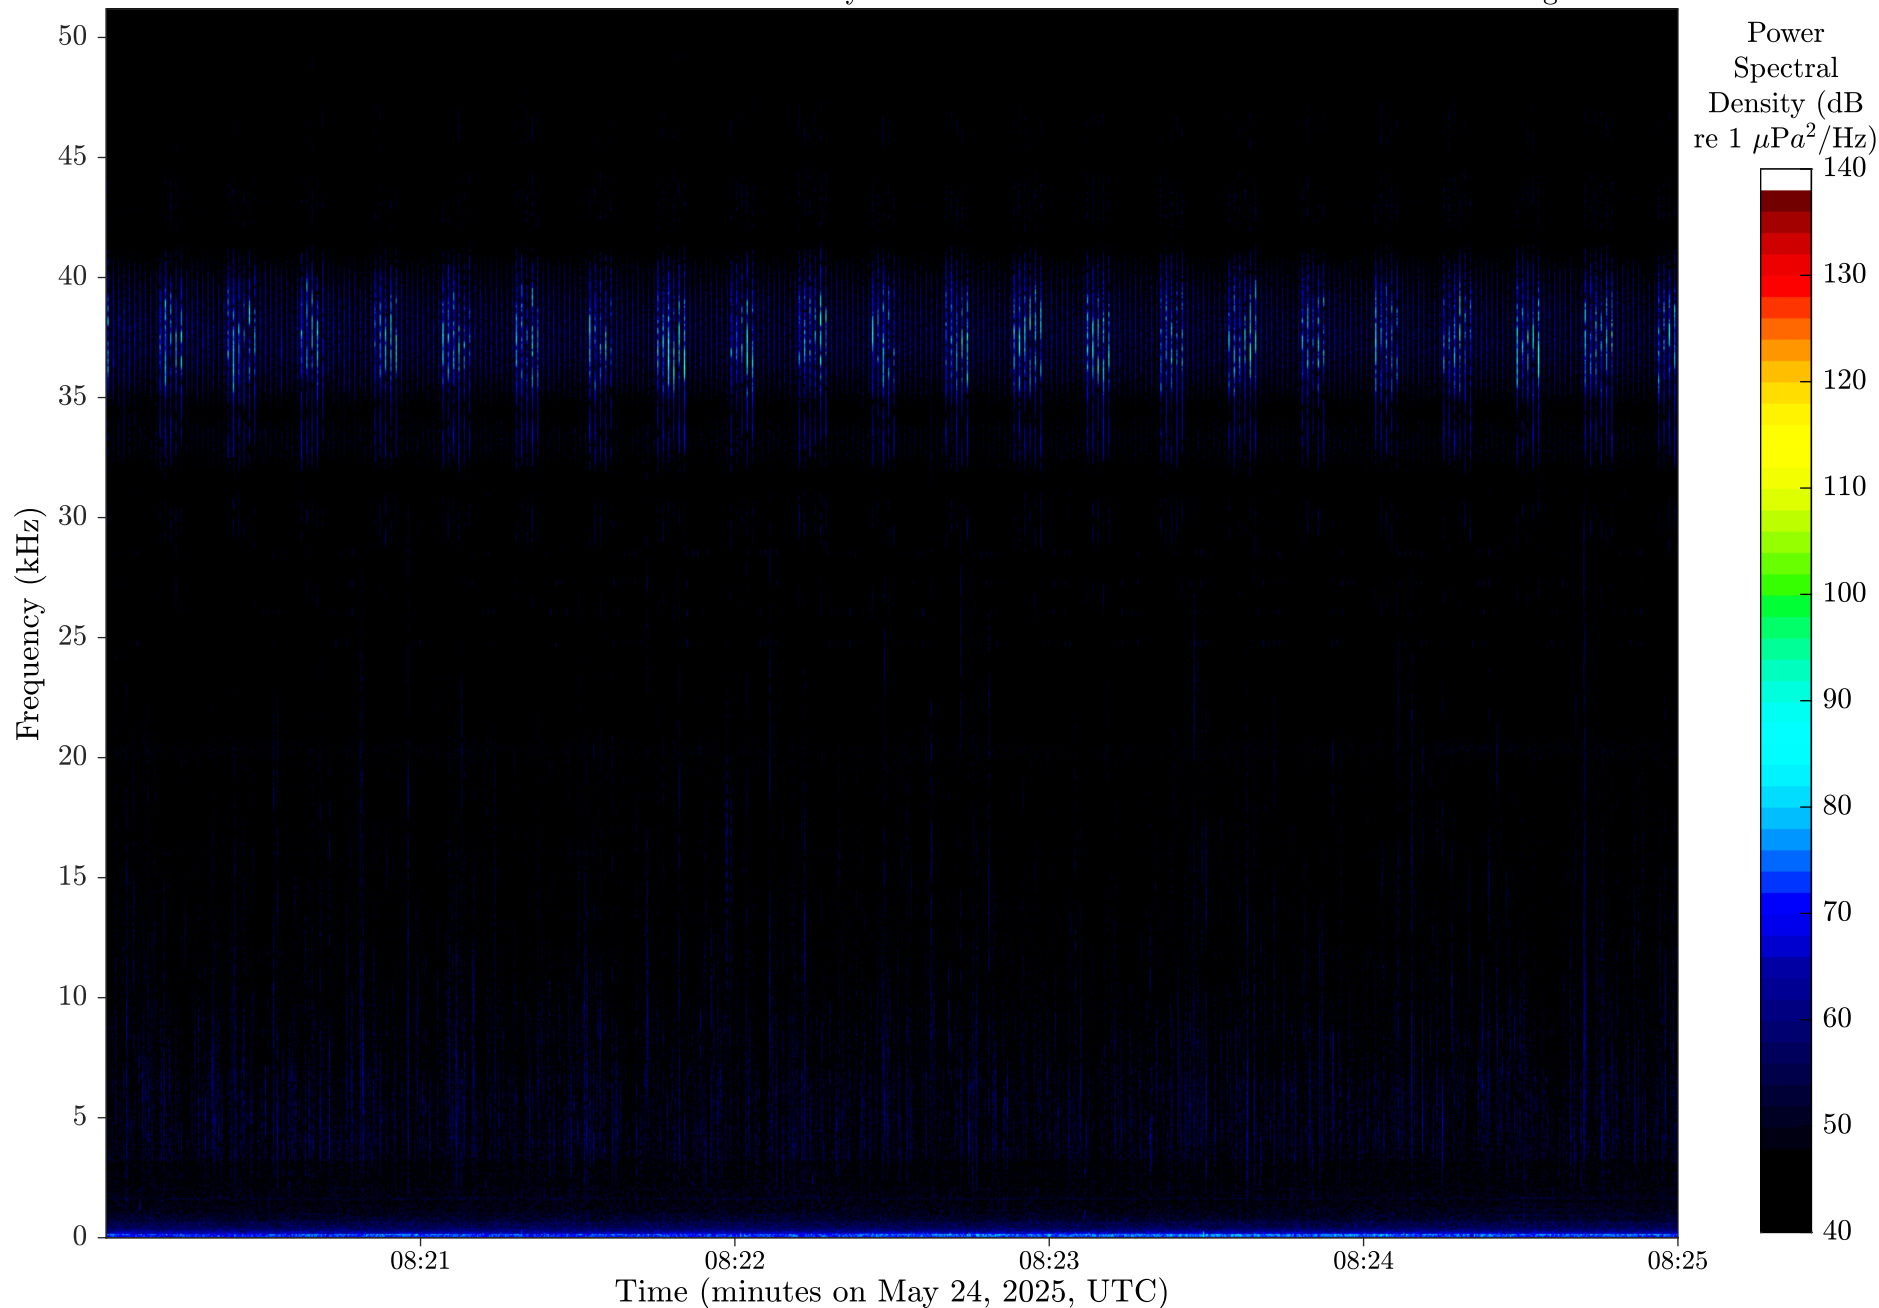


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:24:20 UTC

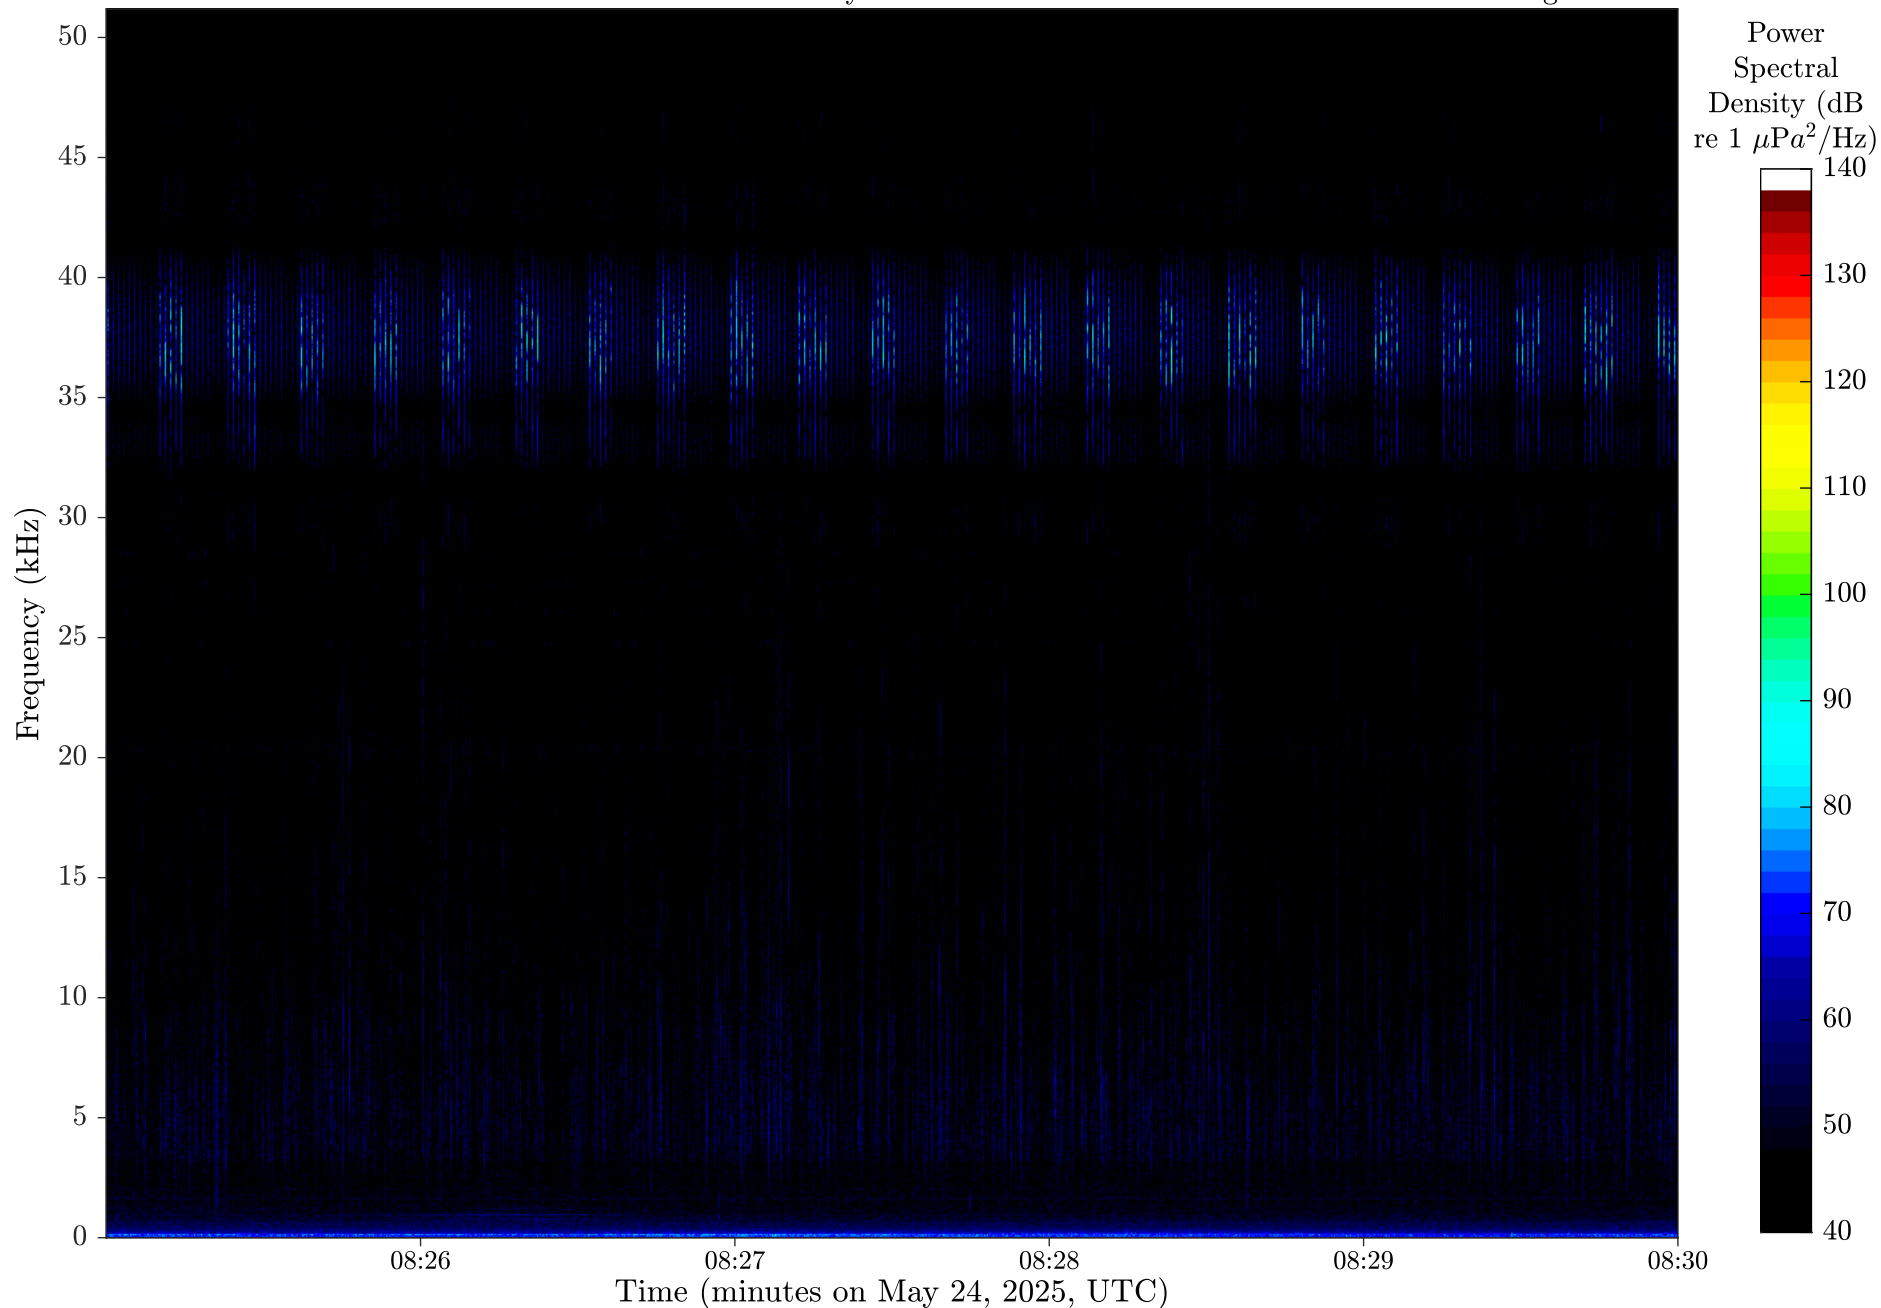


Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:24:27 UTC

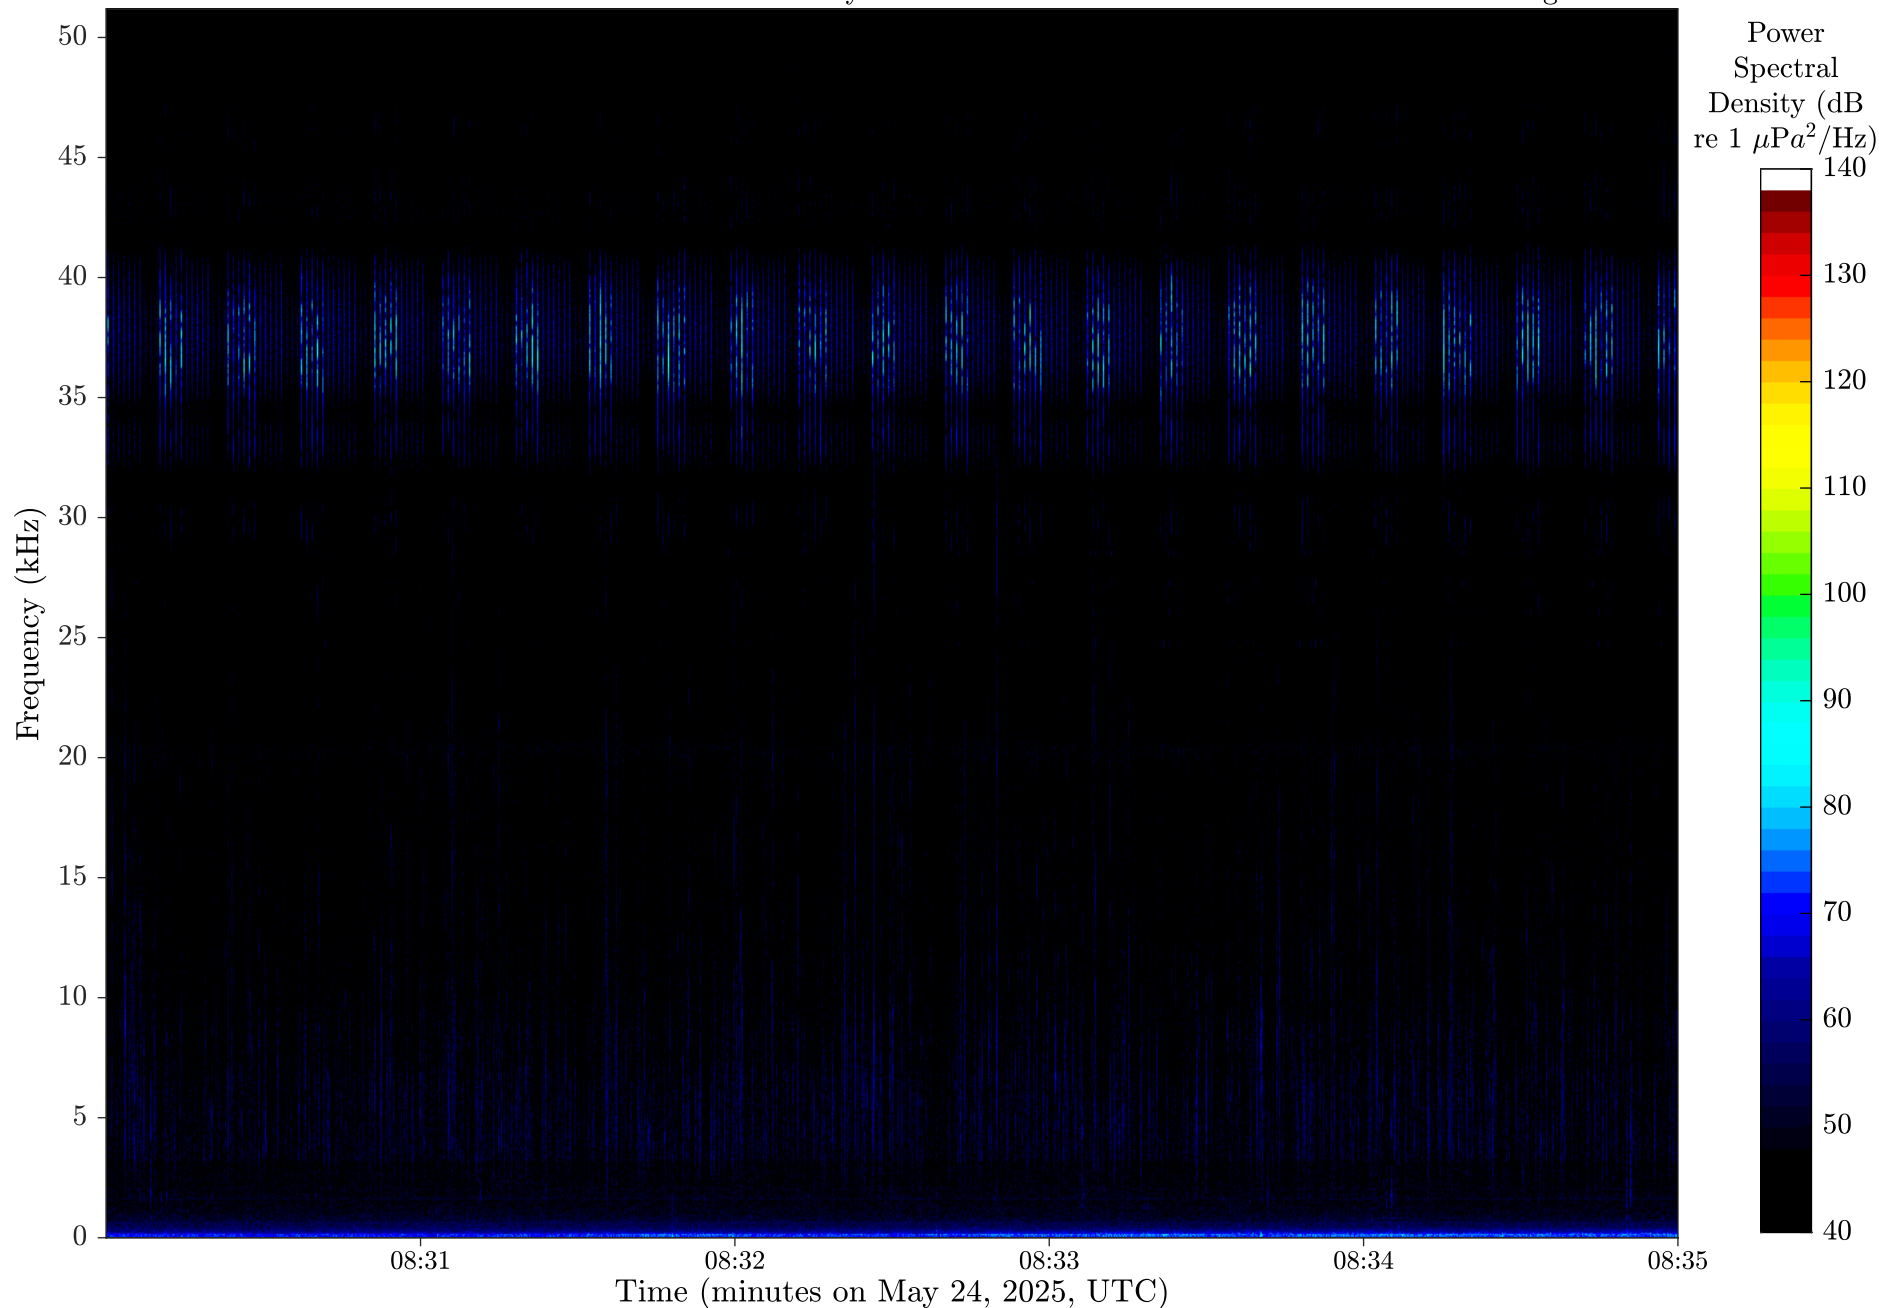


Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:24:34 UTC

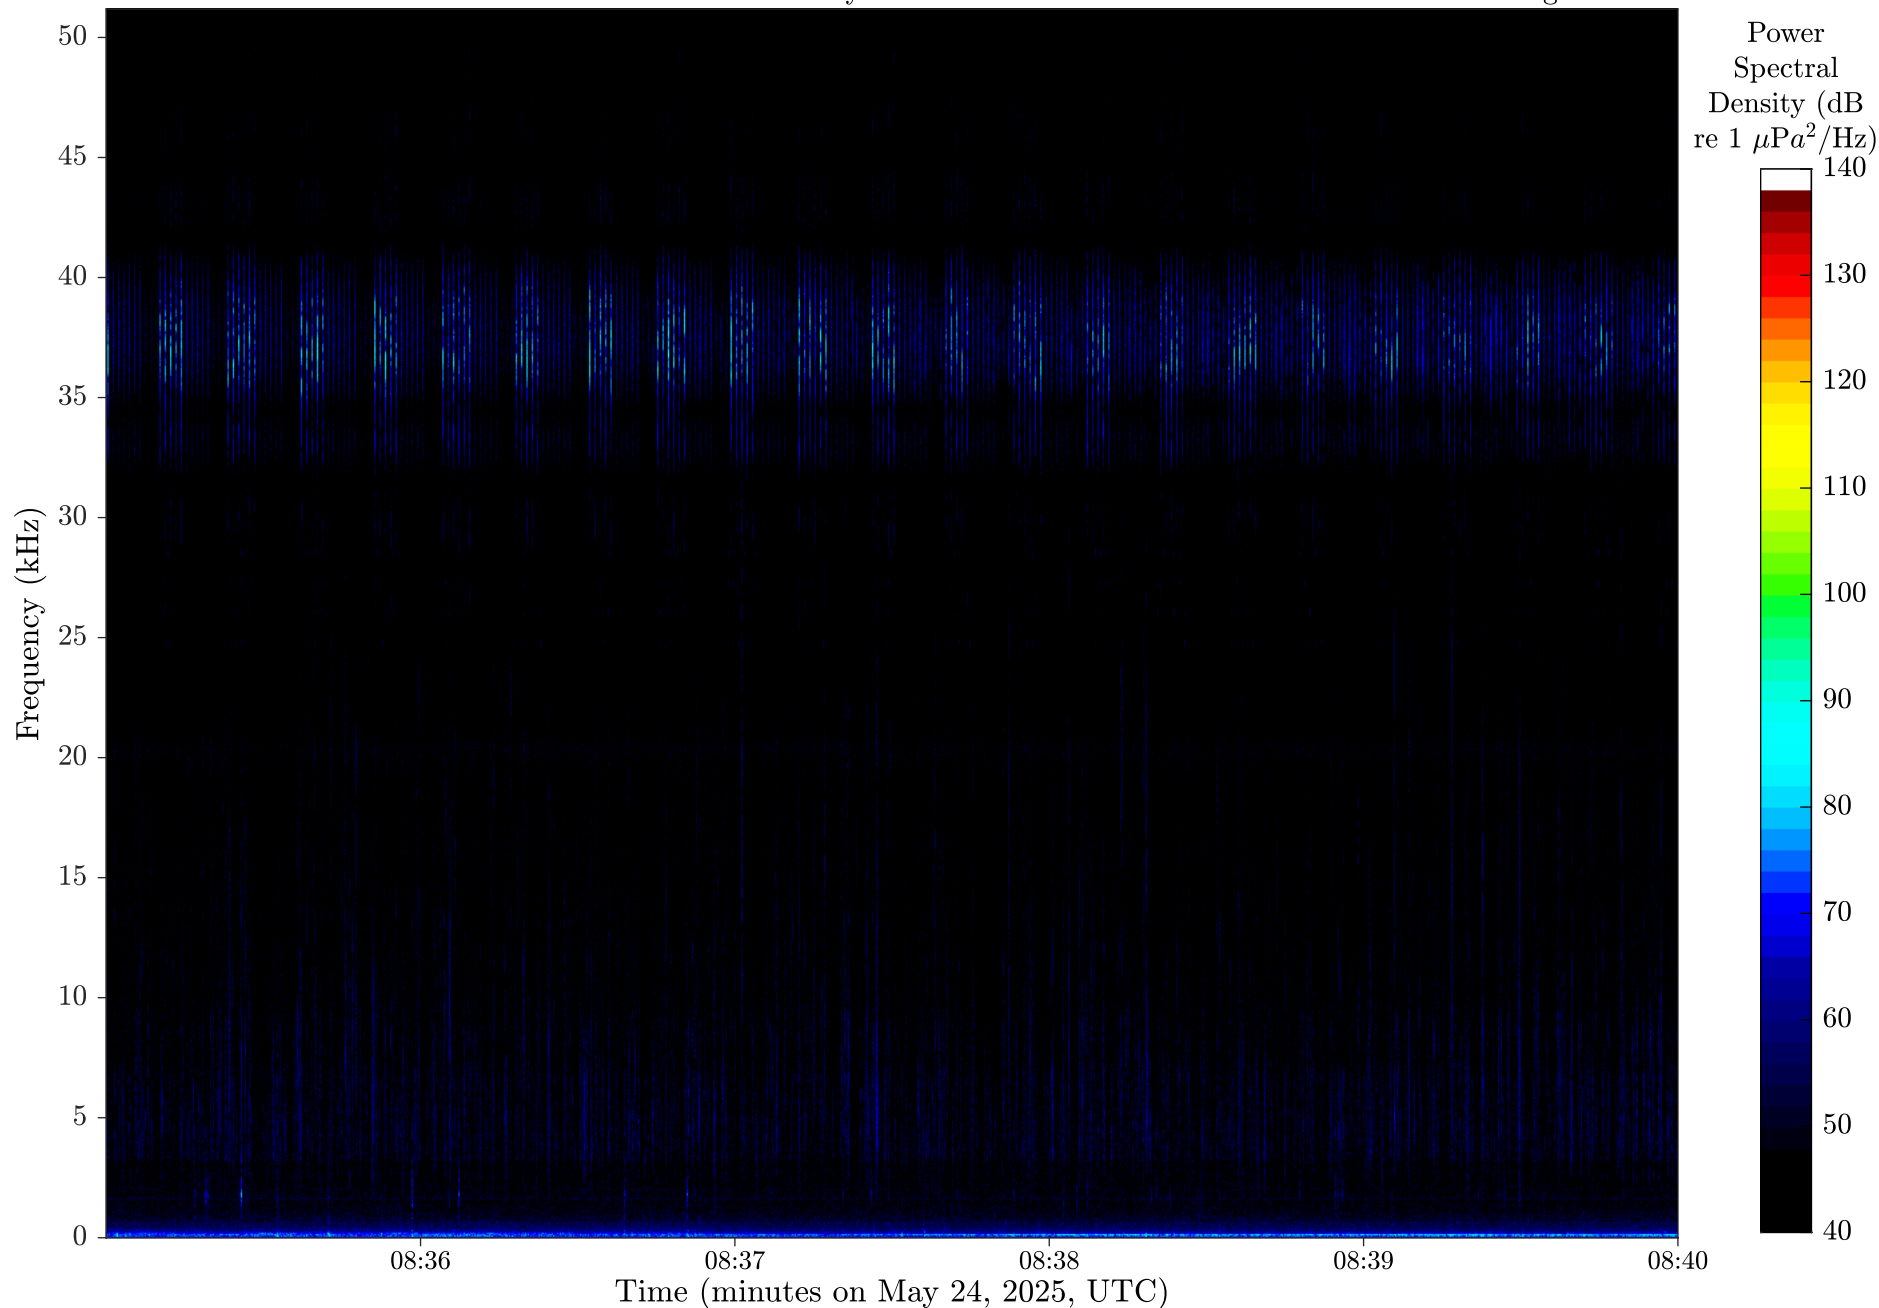


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:24:41 UTC

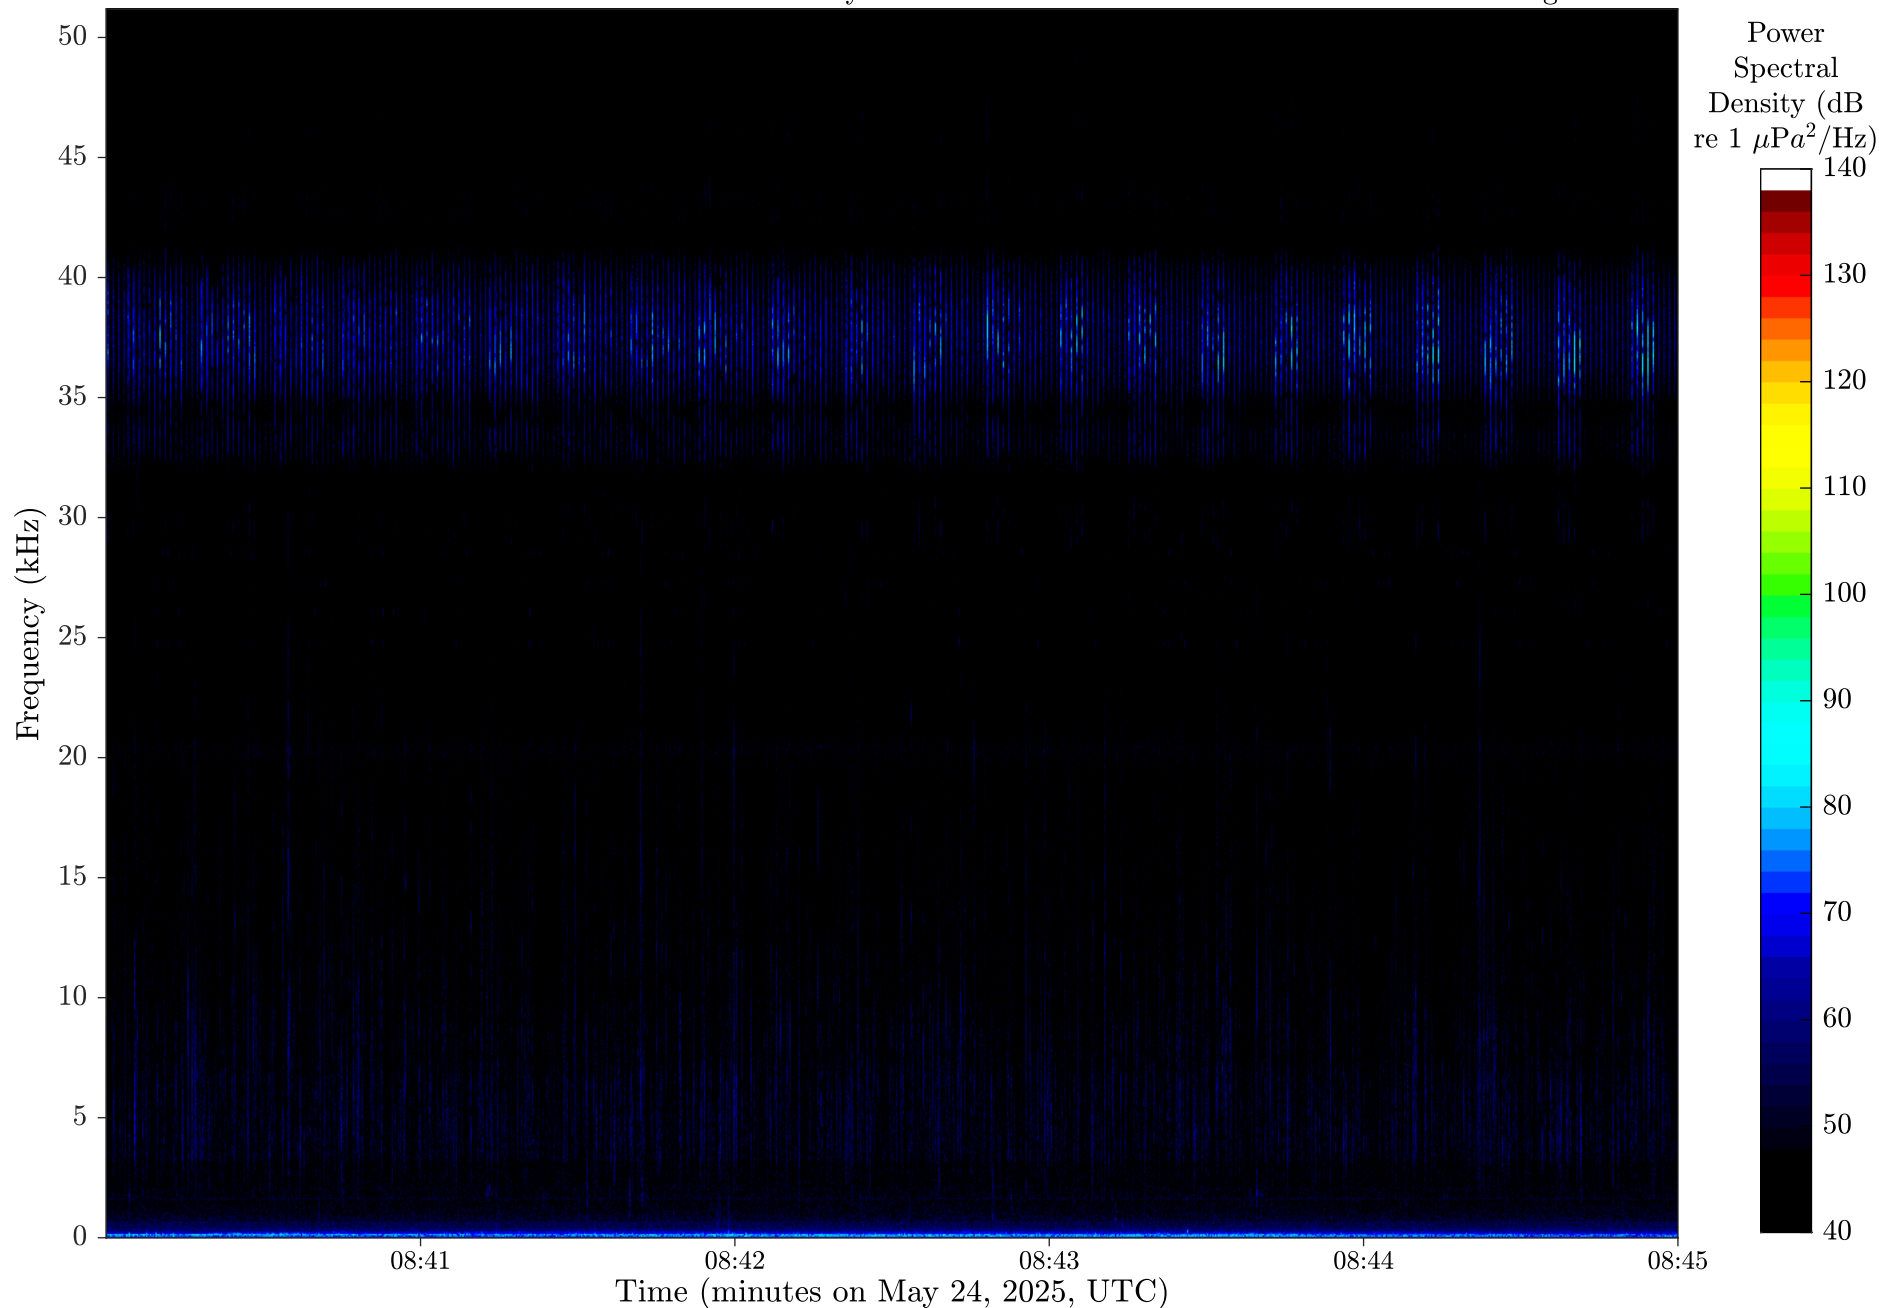


Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:24:48 UTC

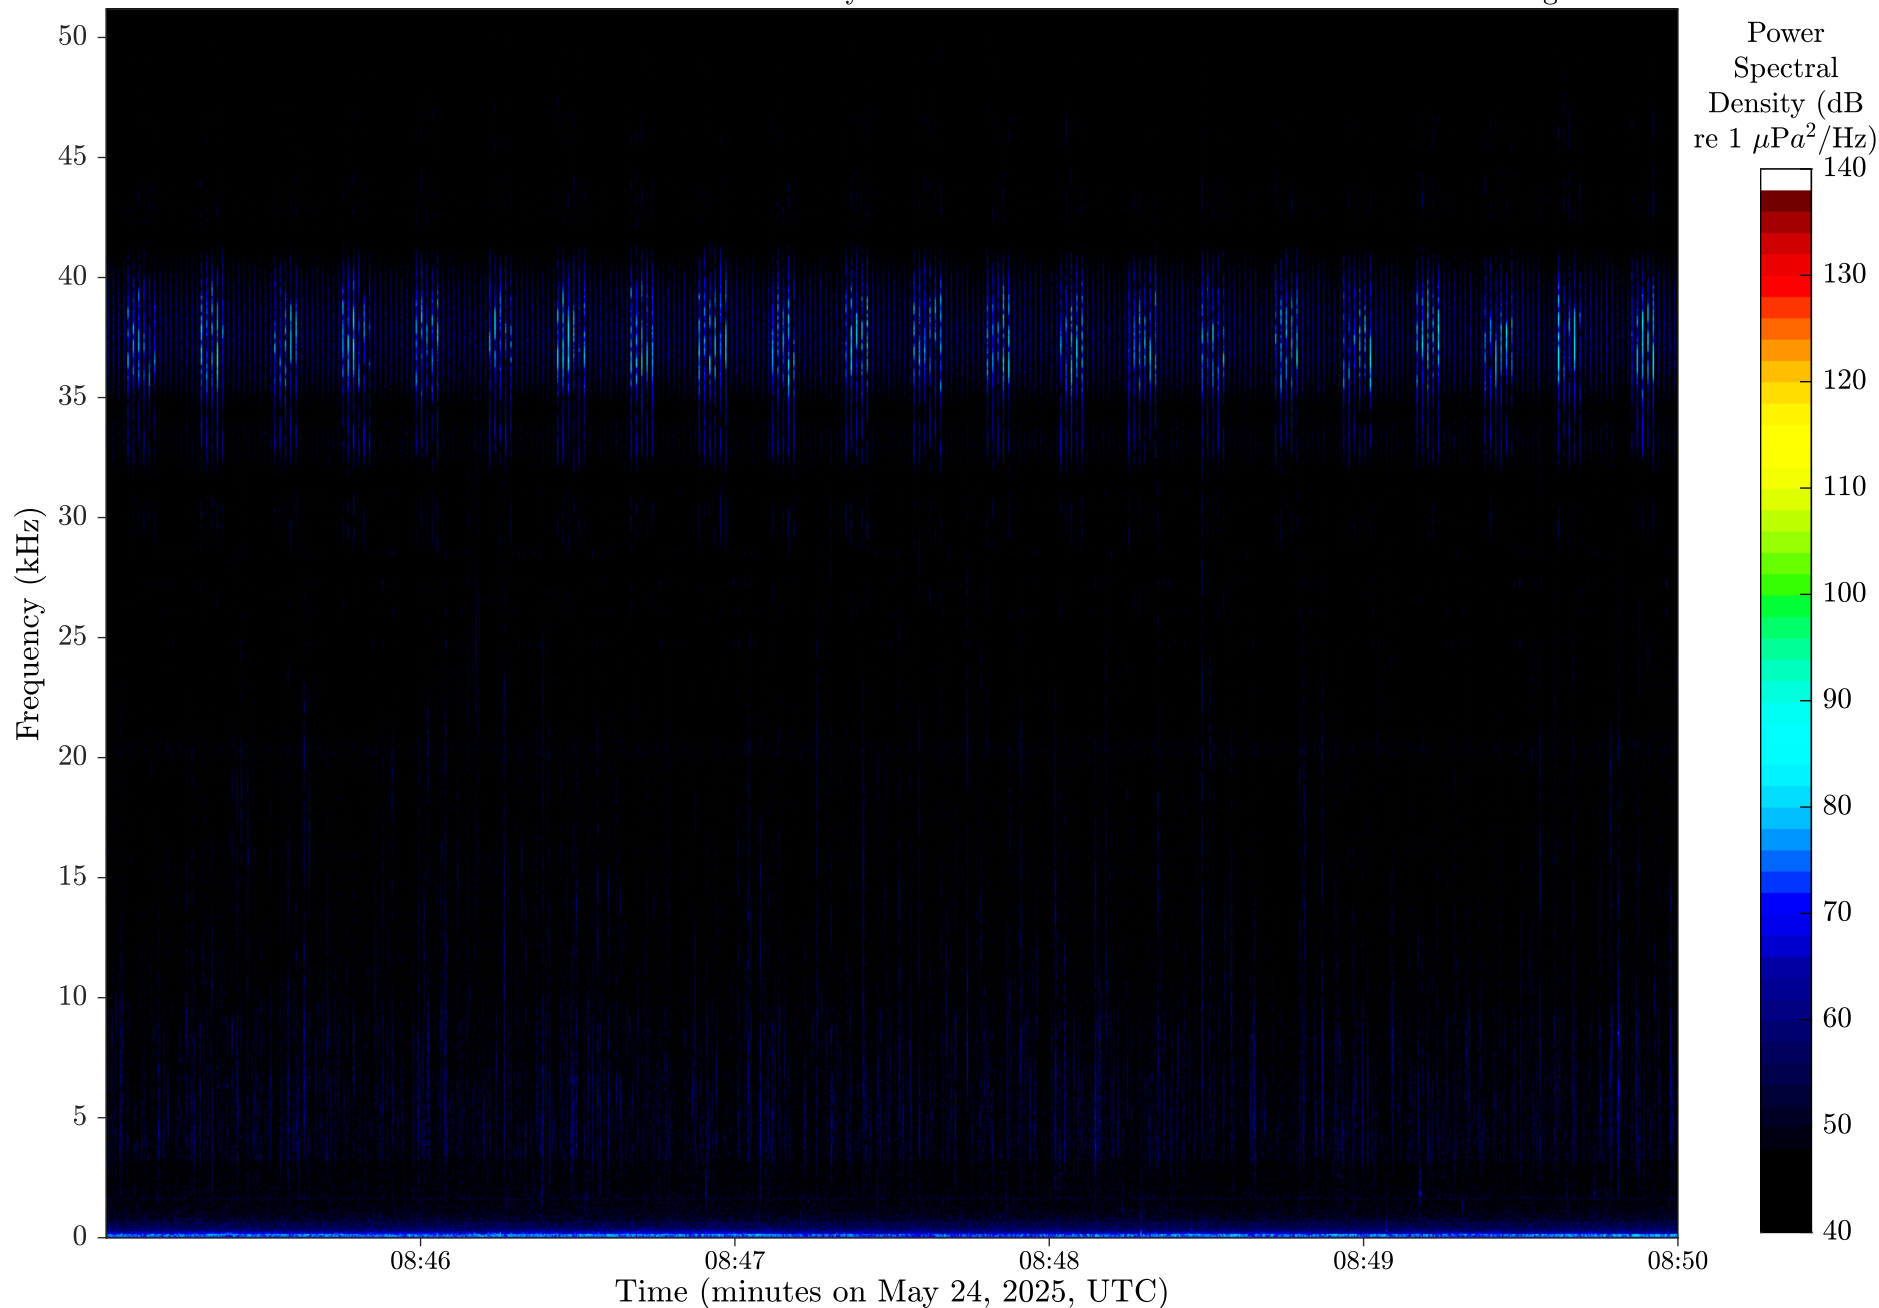


Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:24:55 UTC

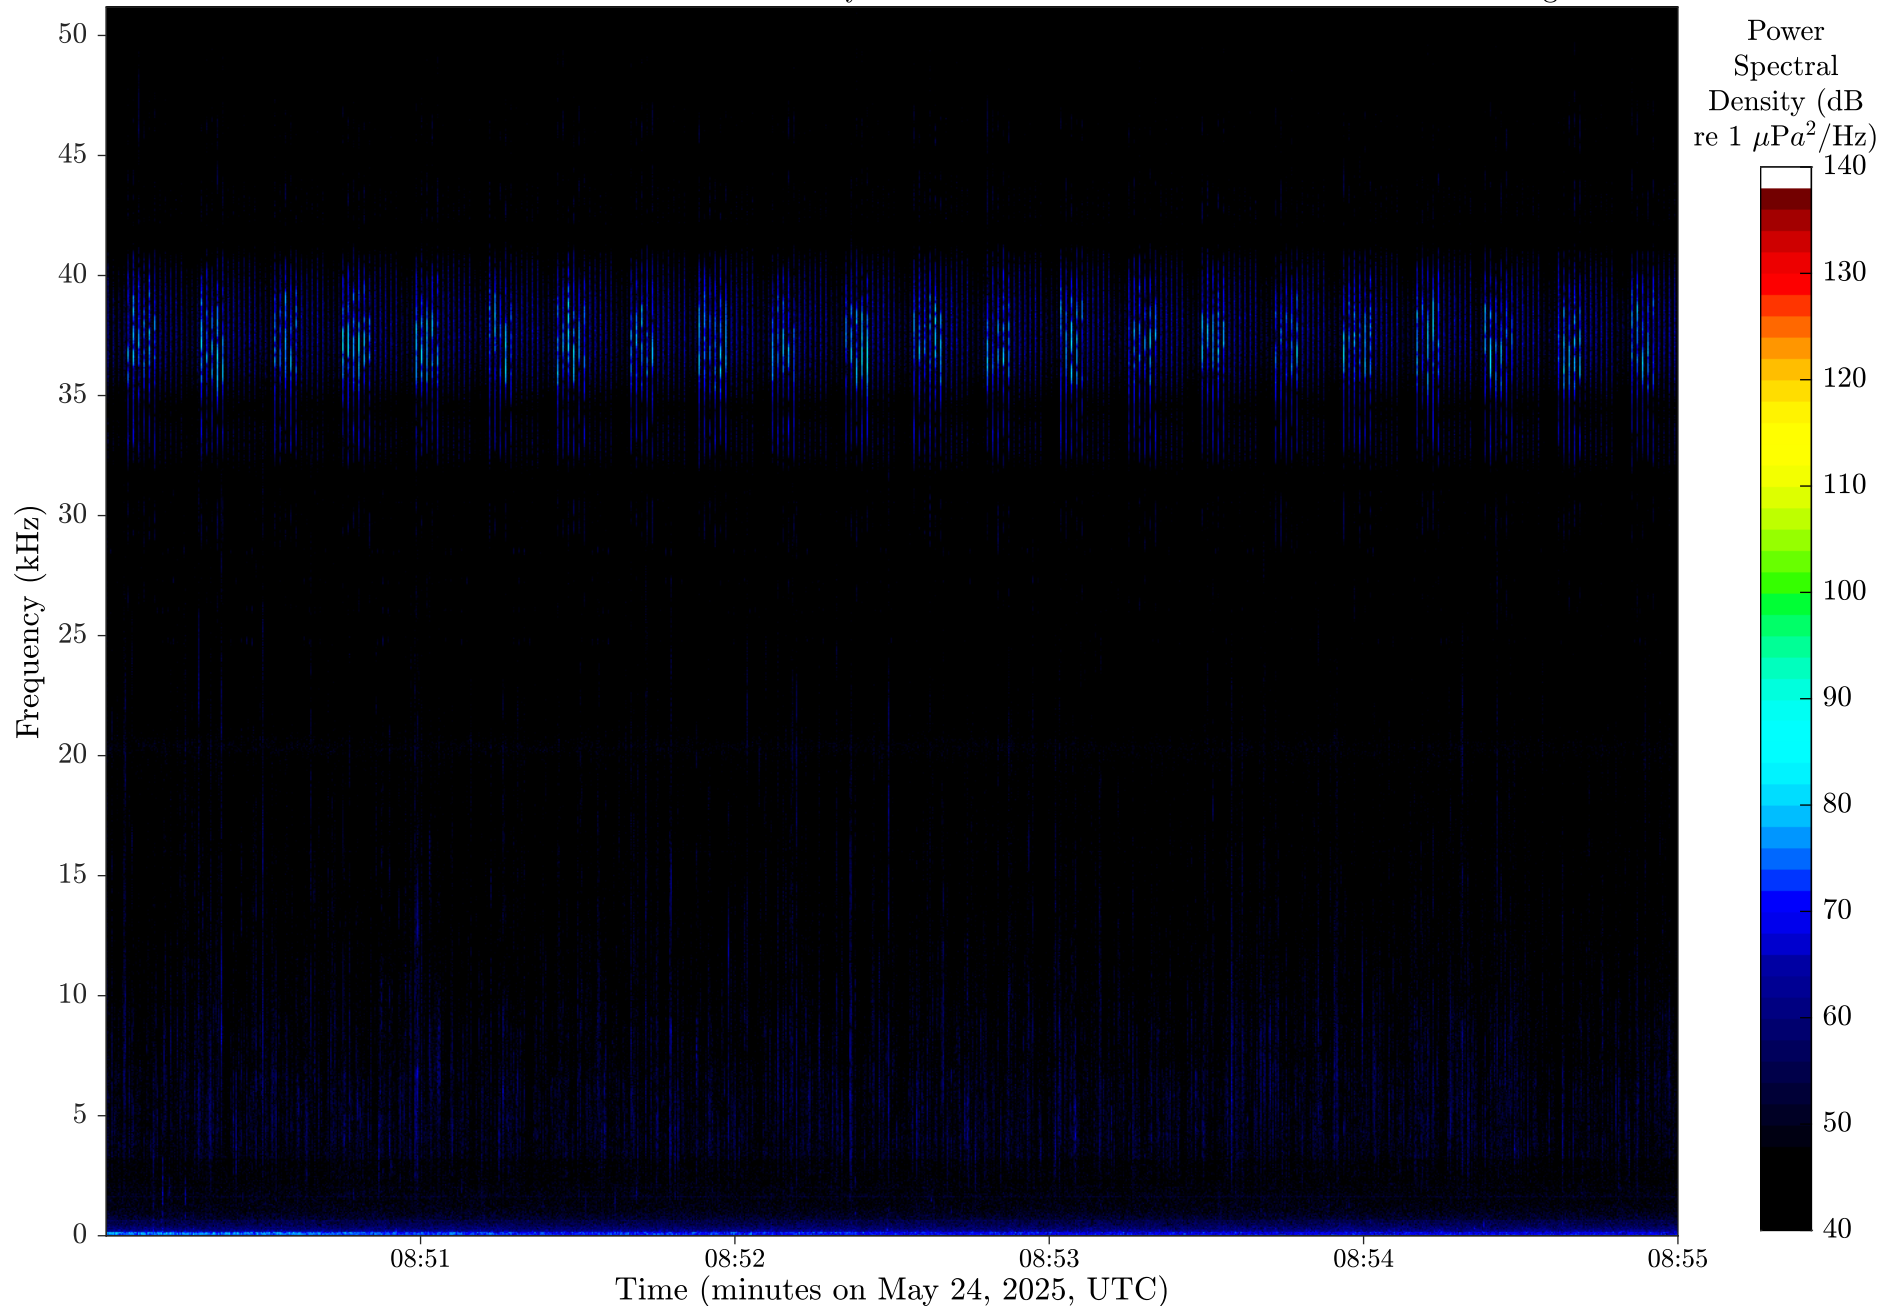


Comments: 36.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:03 UTC

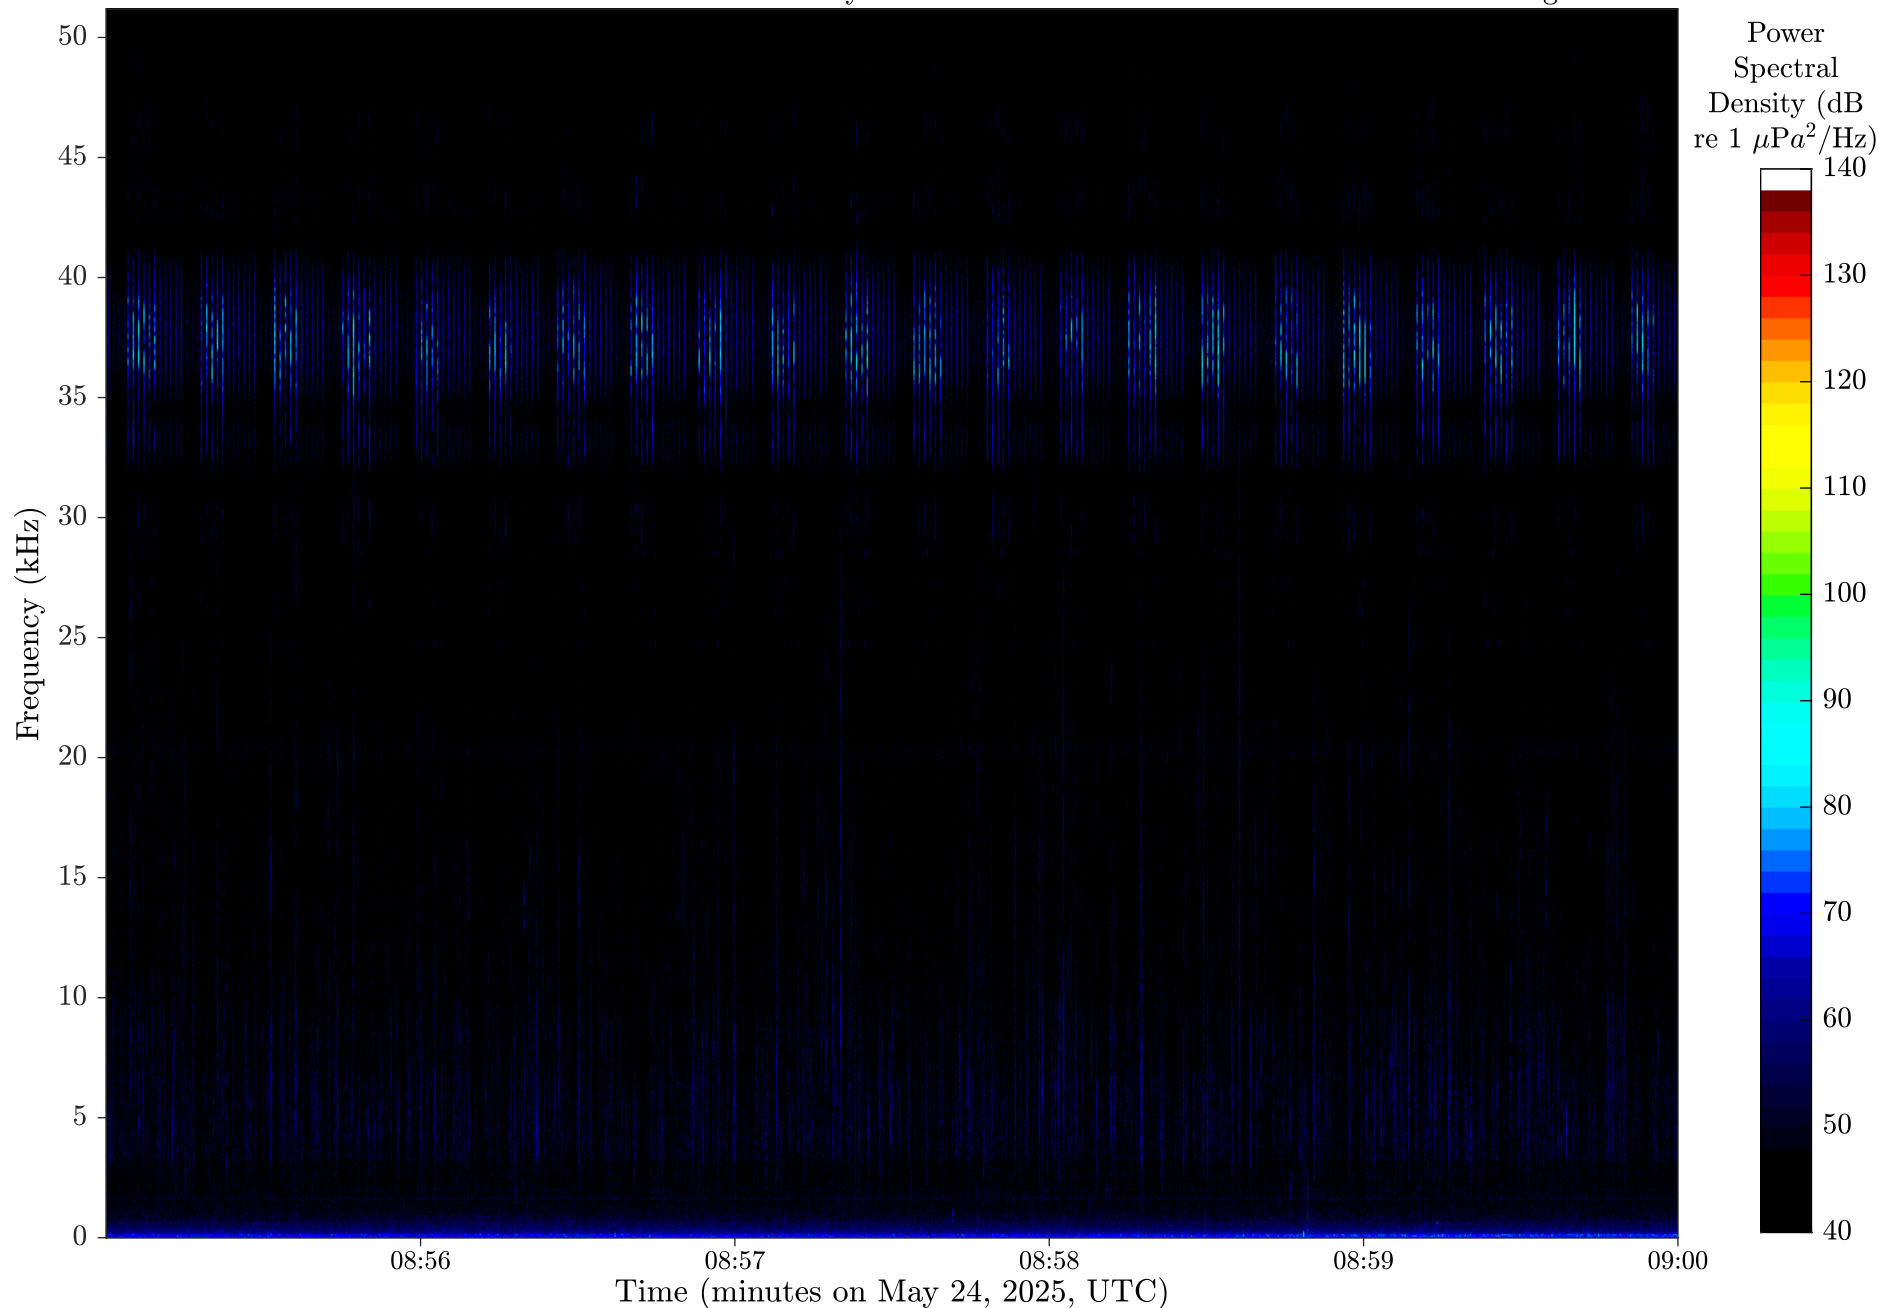


Comments: 36.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:10 UTC

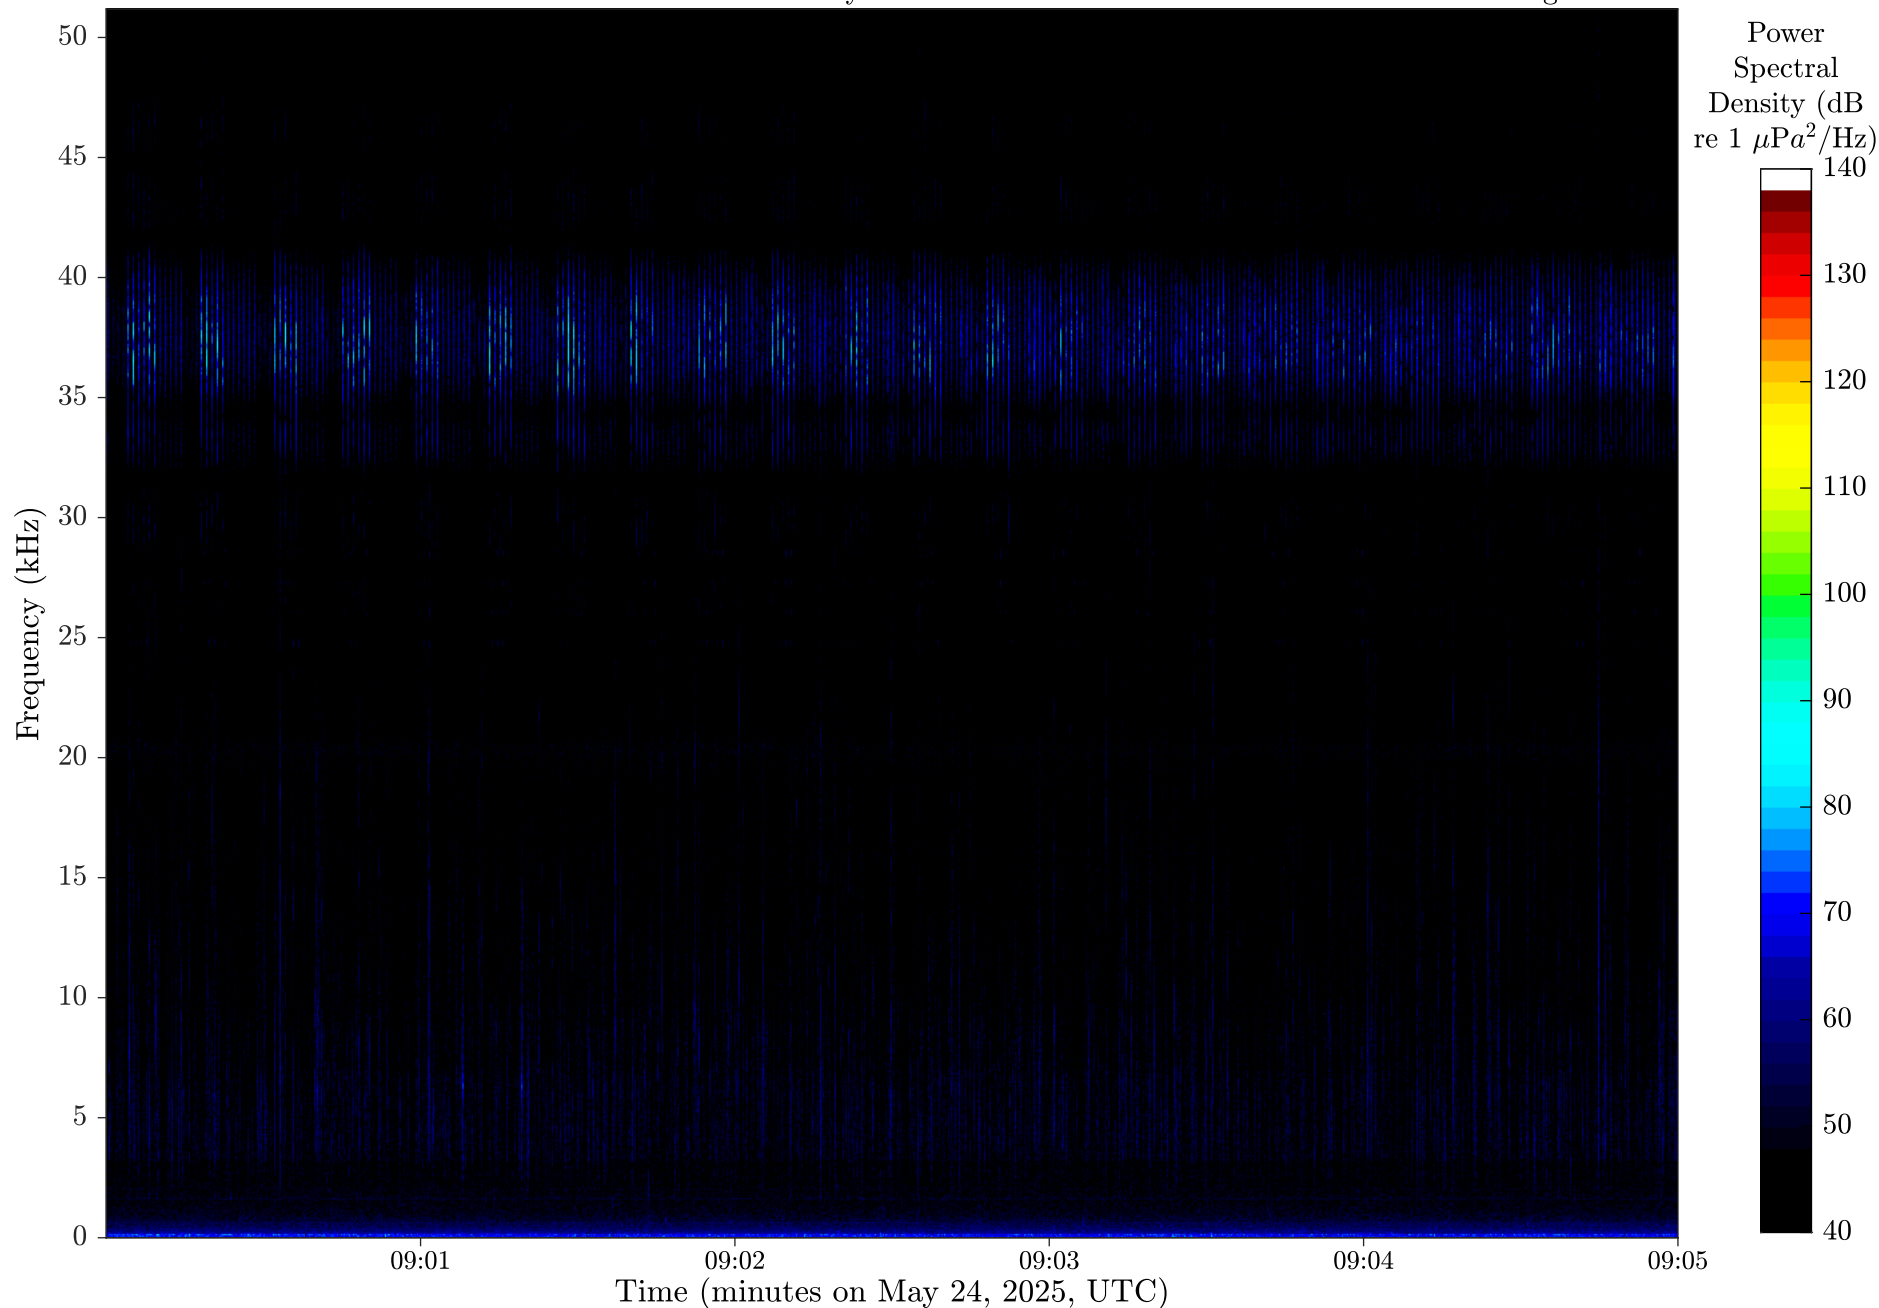


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:25:18 UTC

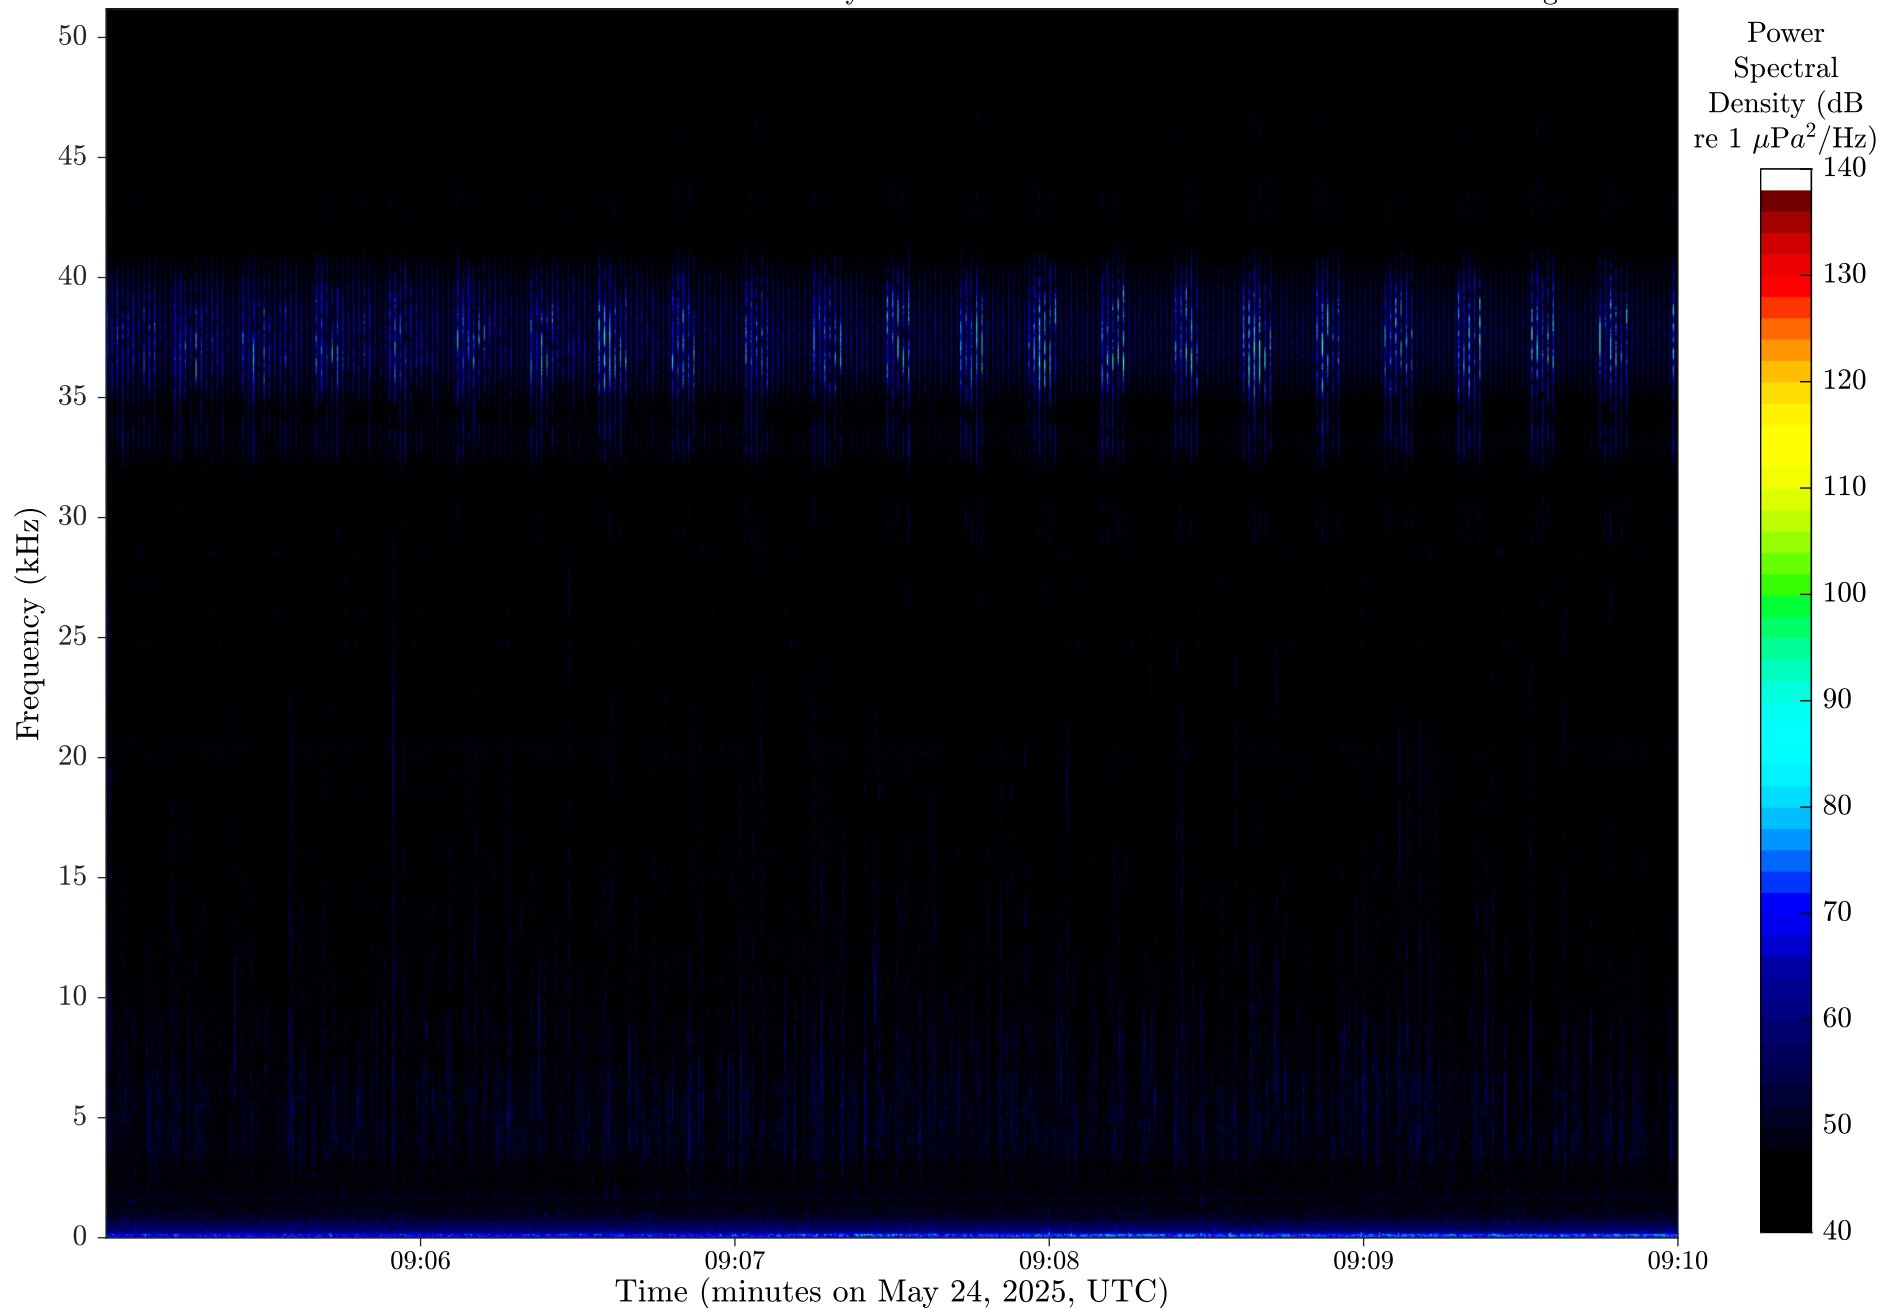

Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:25:25 UTC

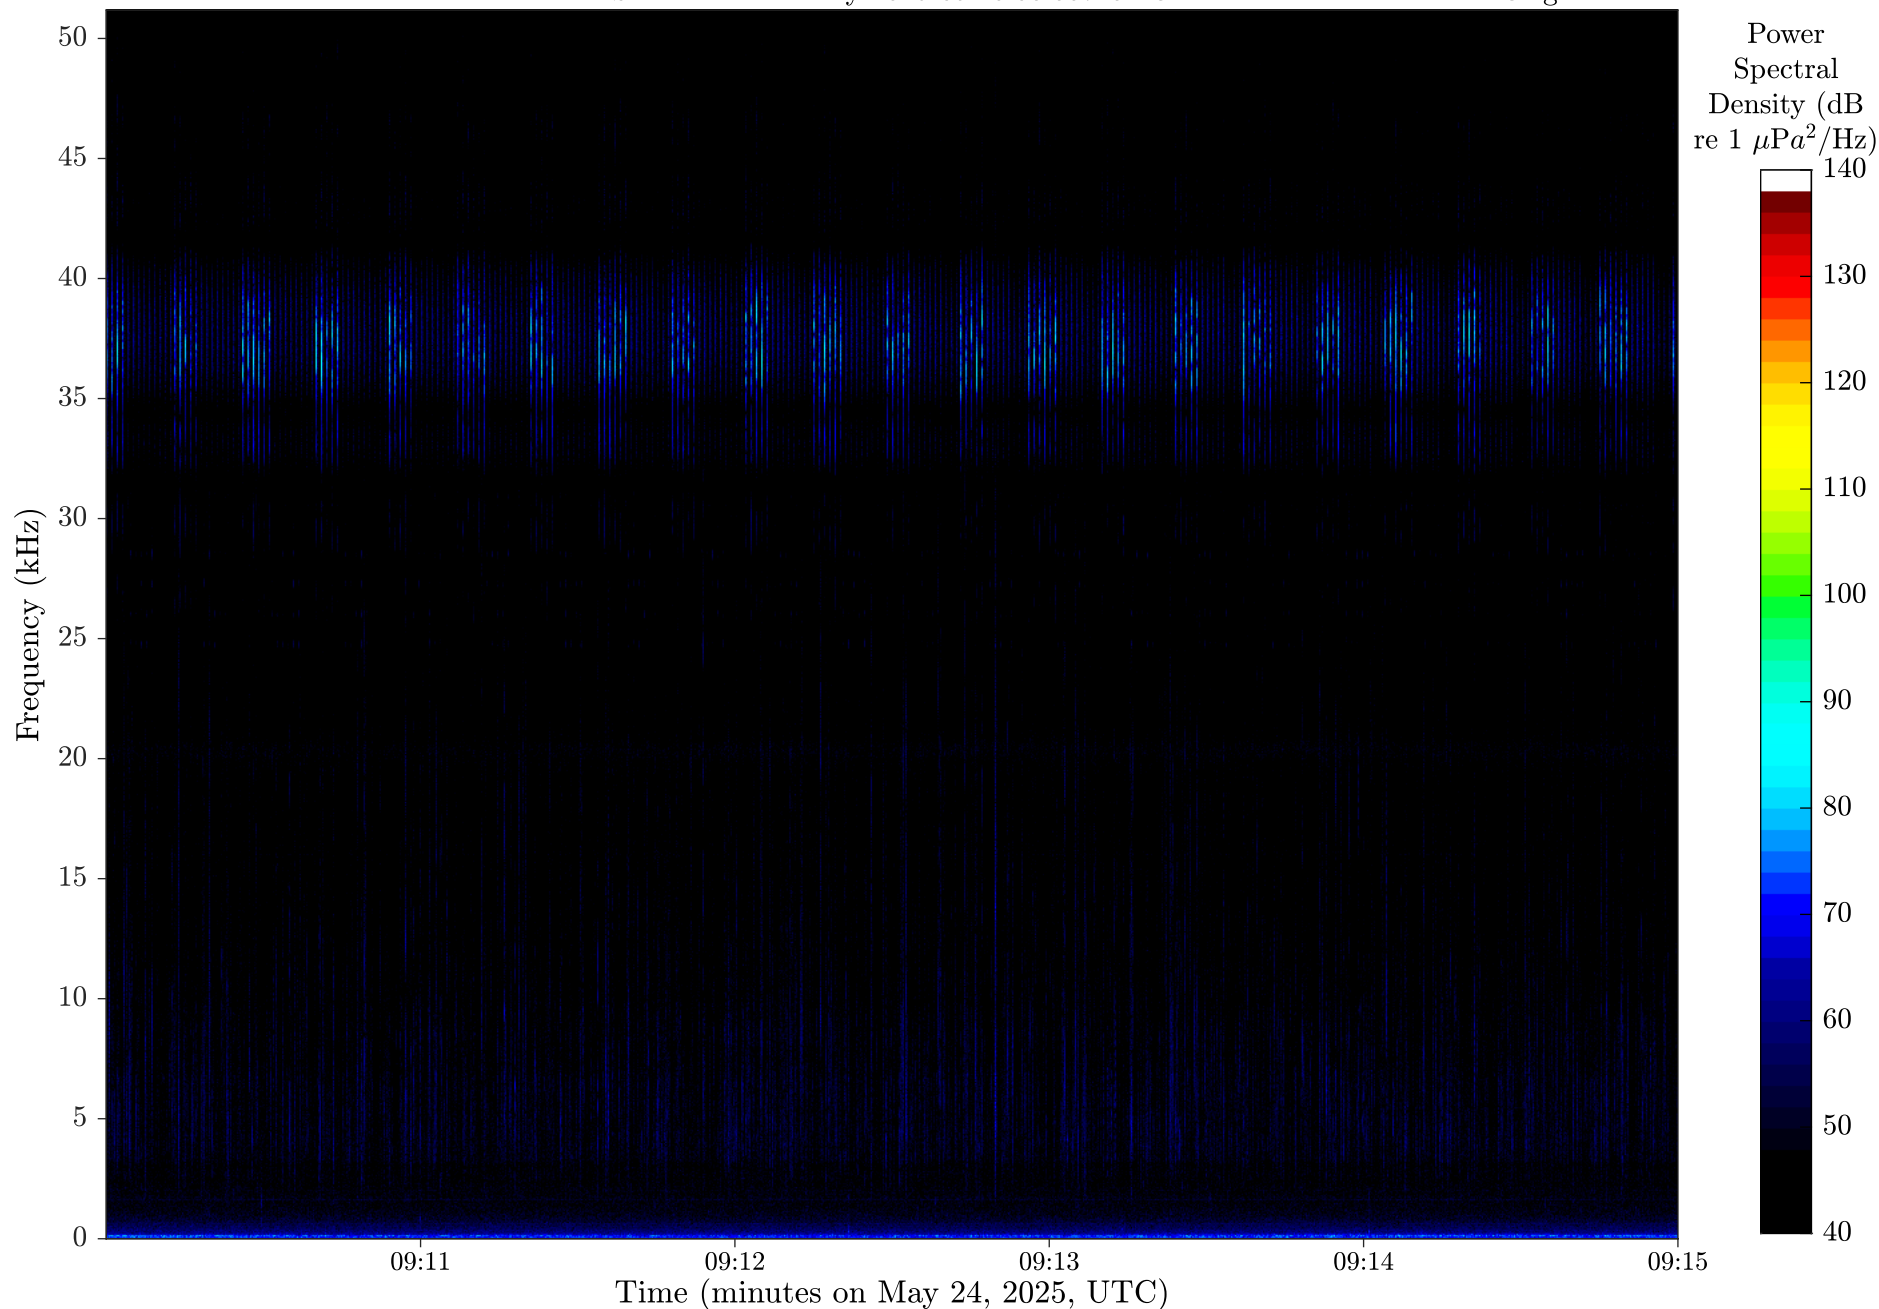

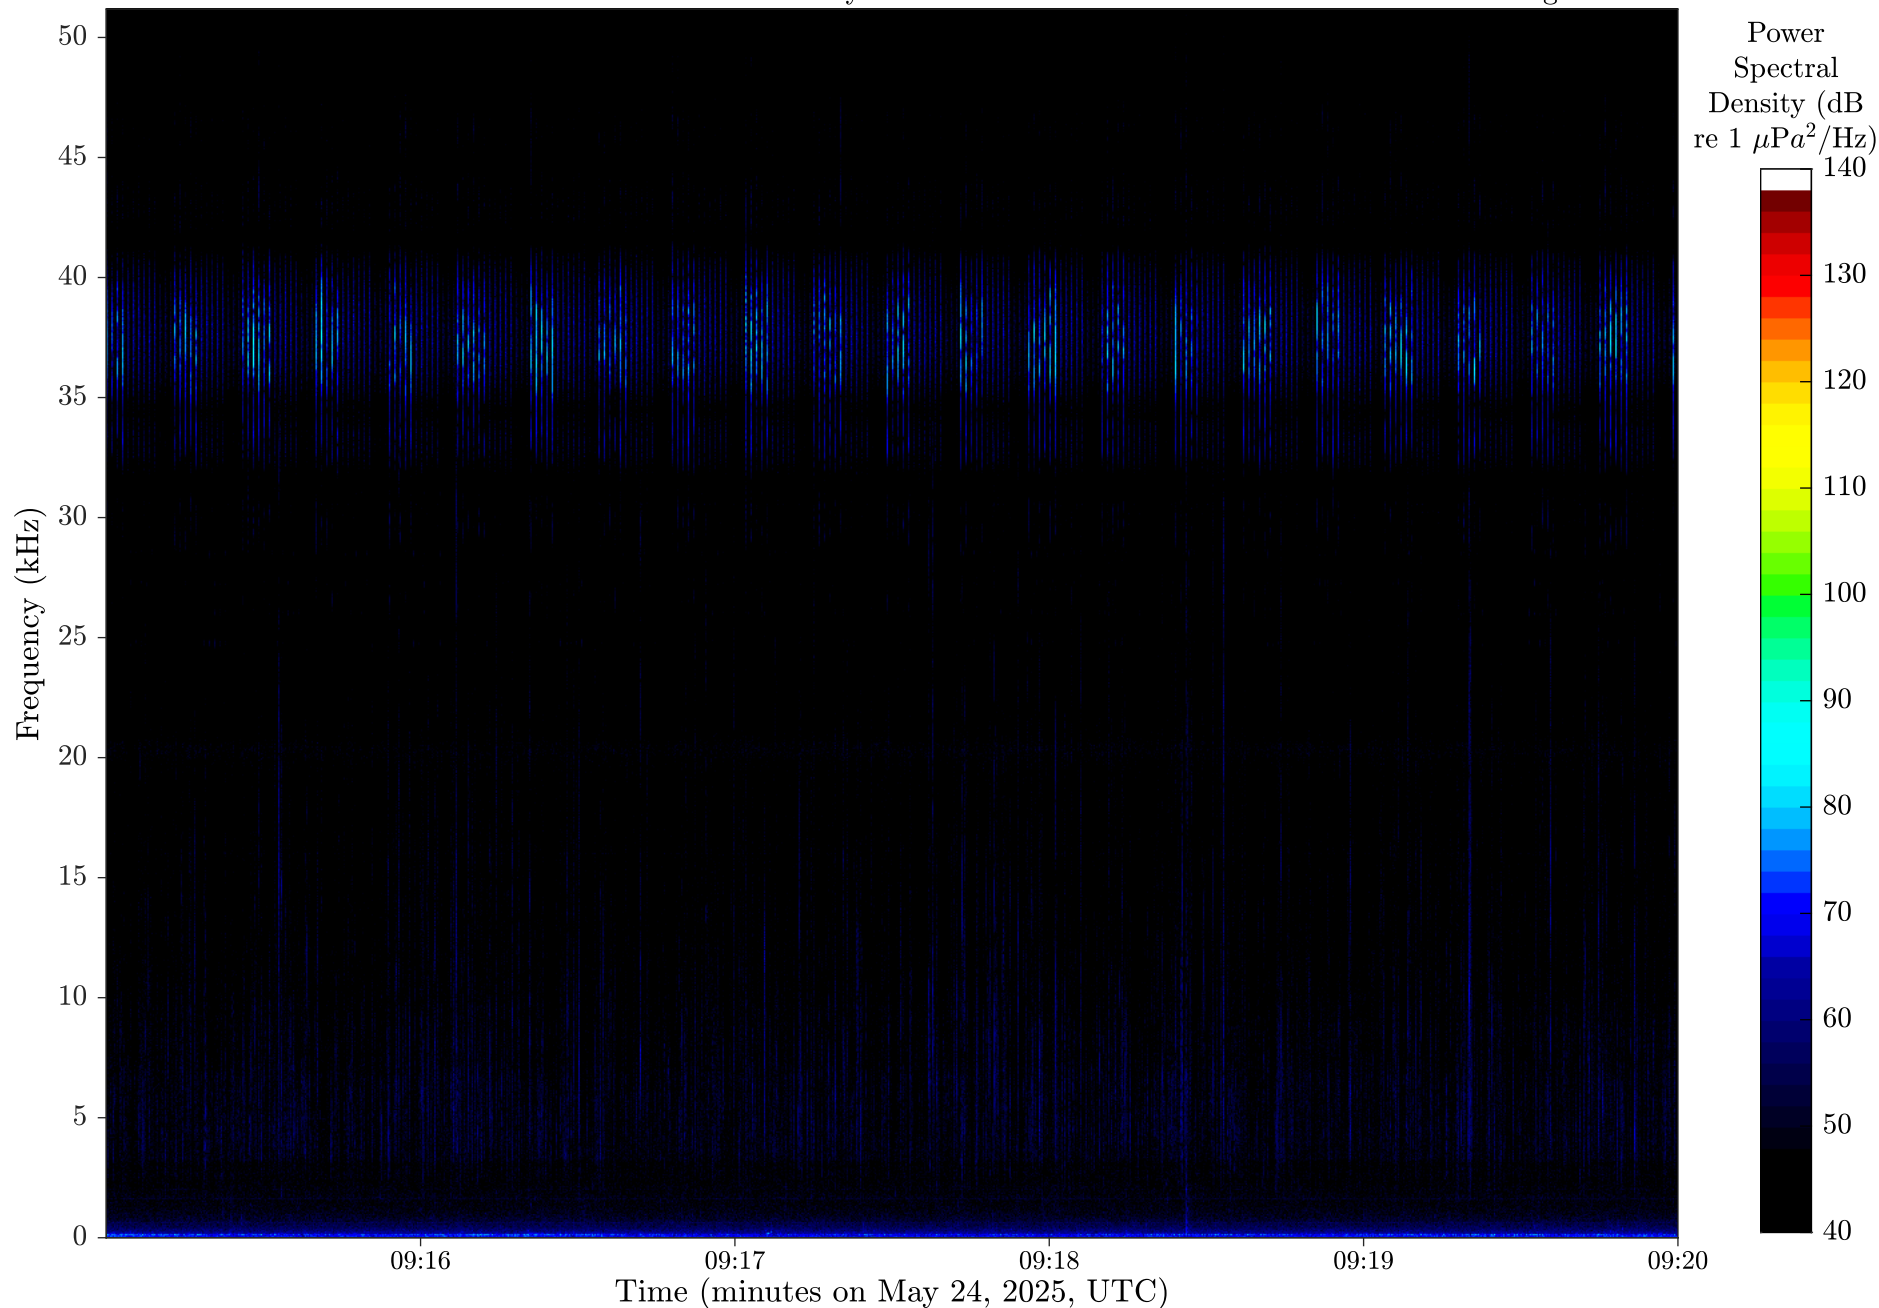


Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:40 UTC

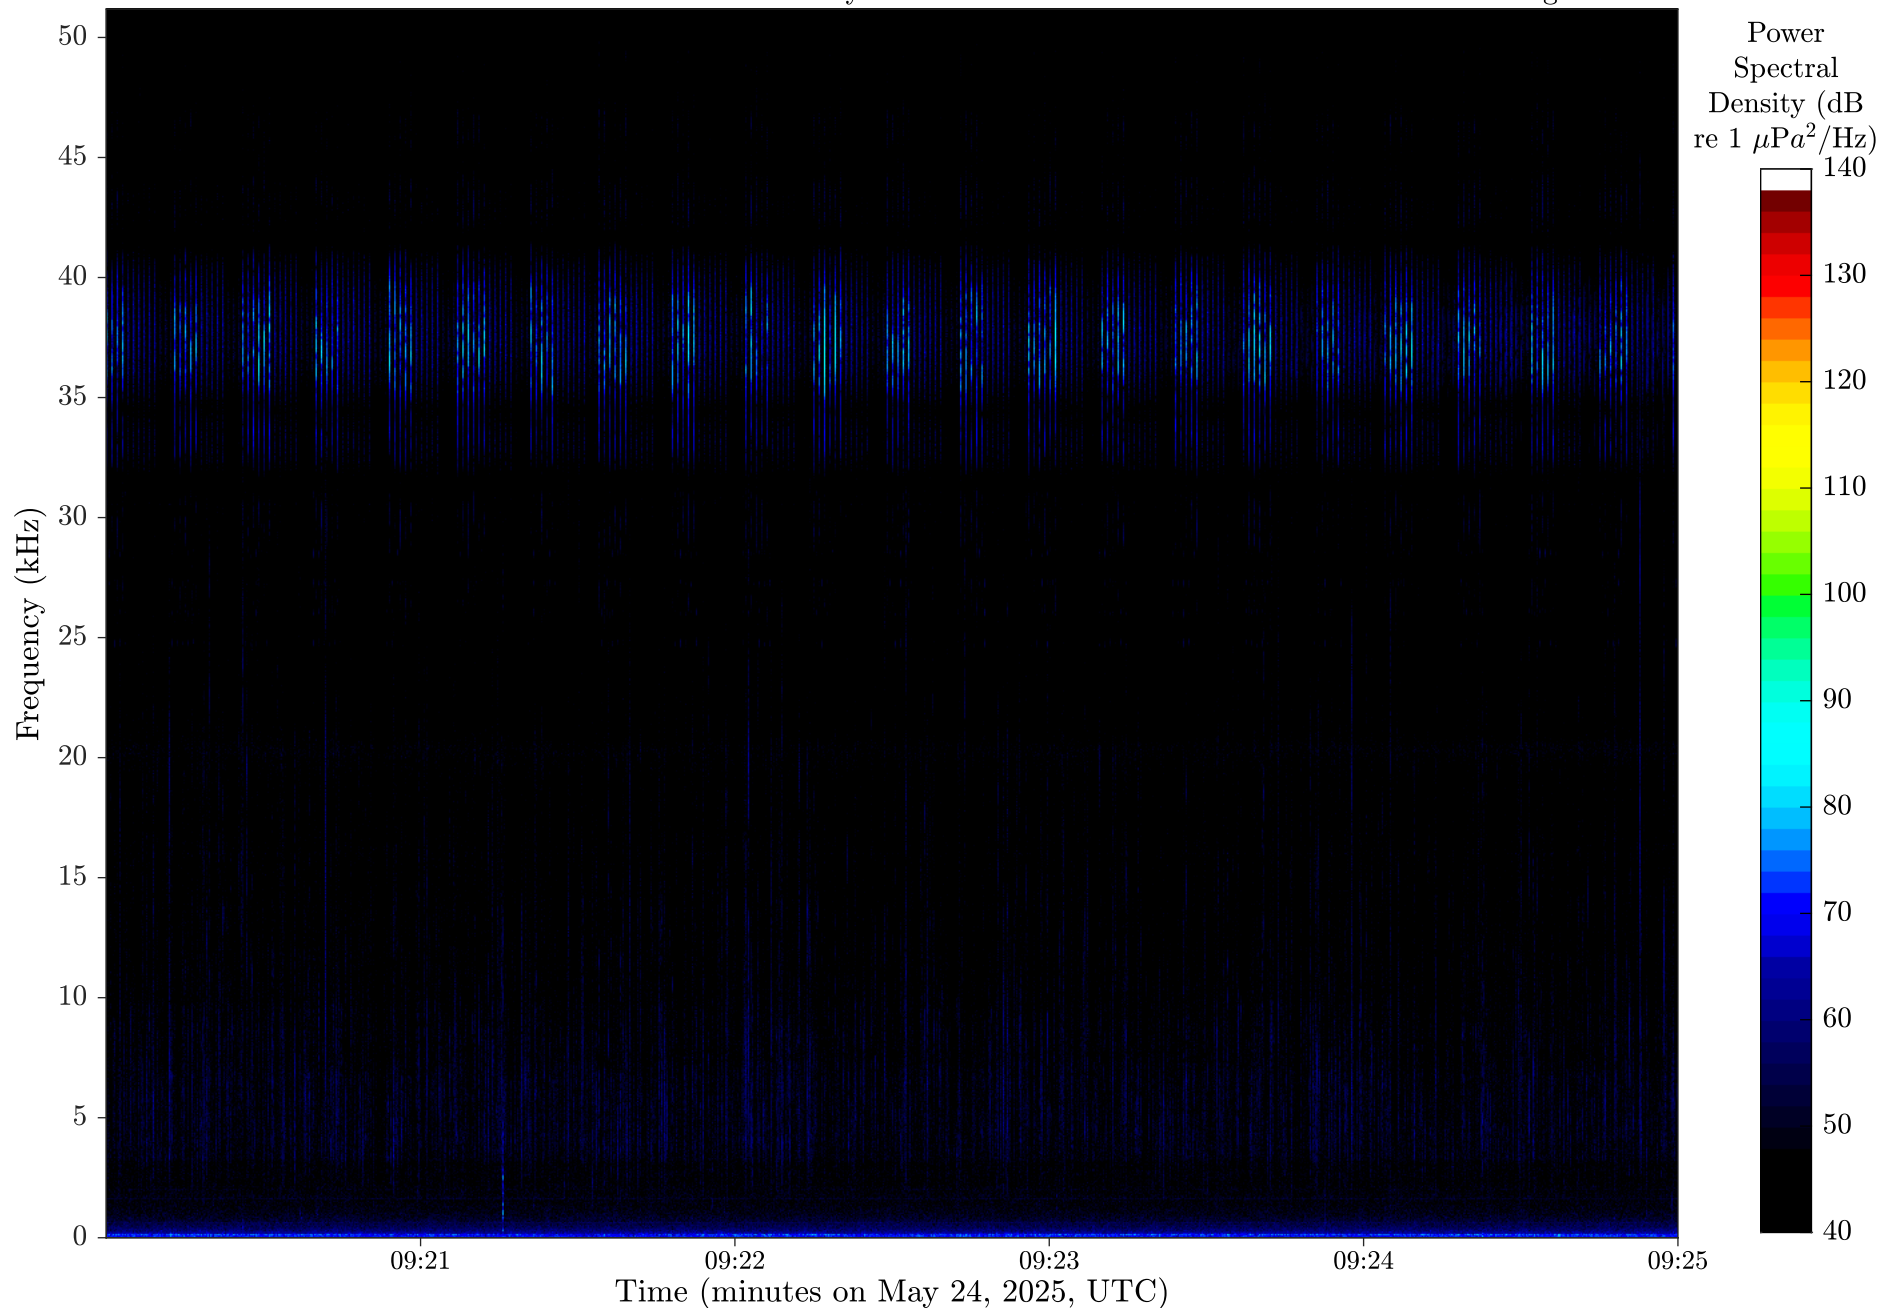


Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:25:47 UTC

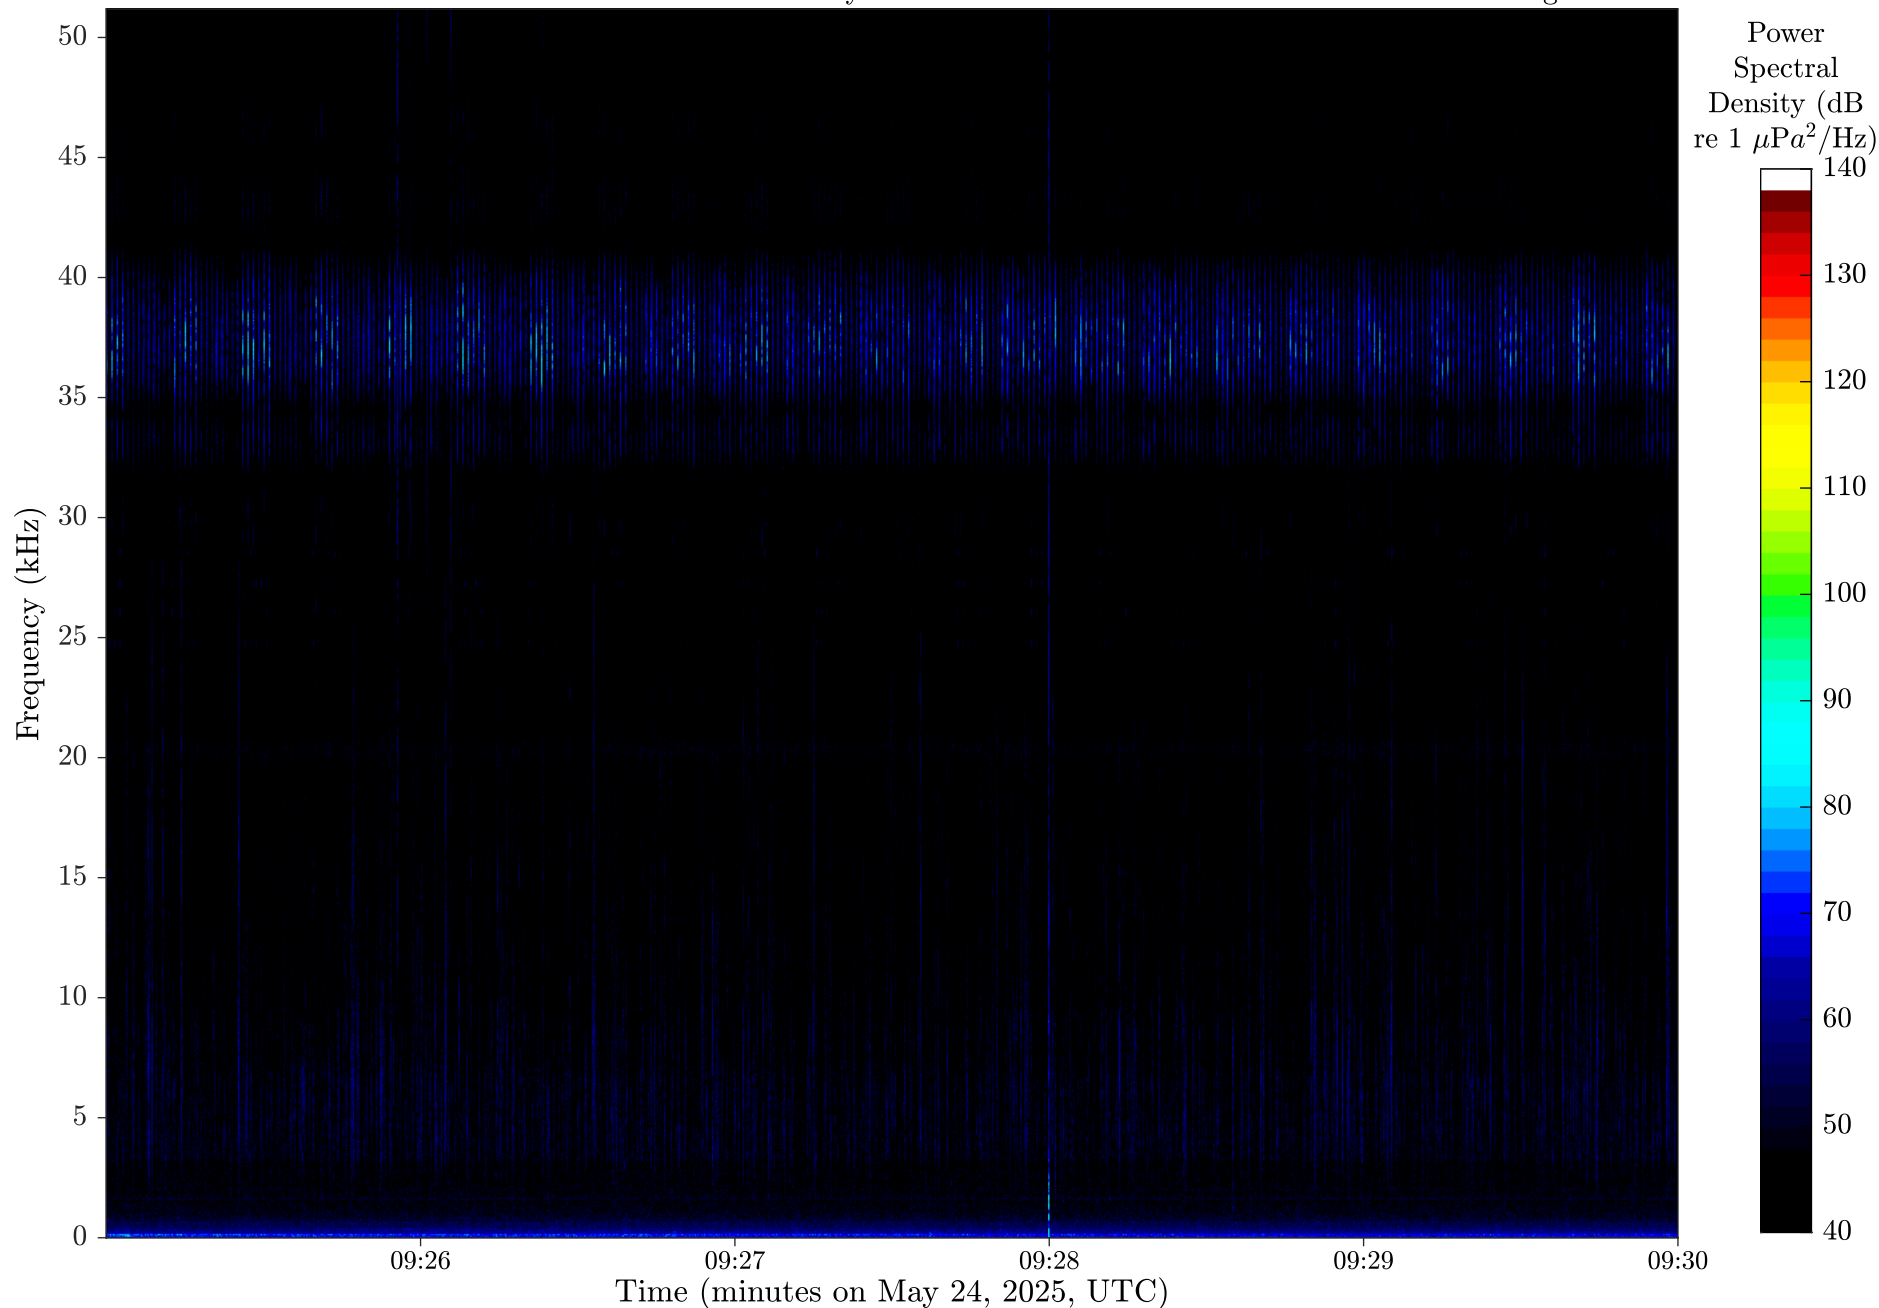

Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:25:54 UTC

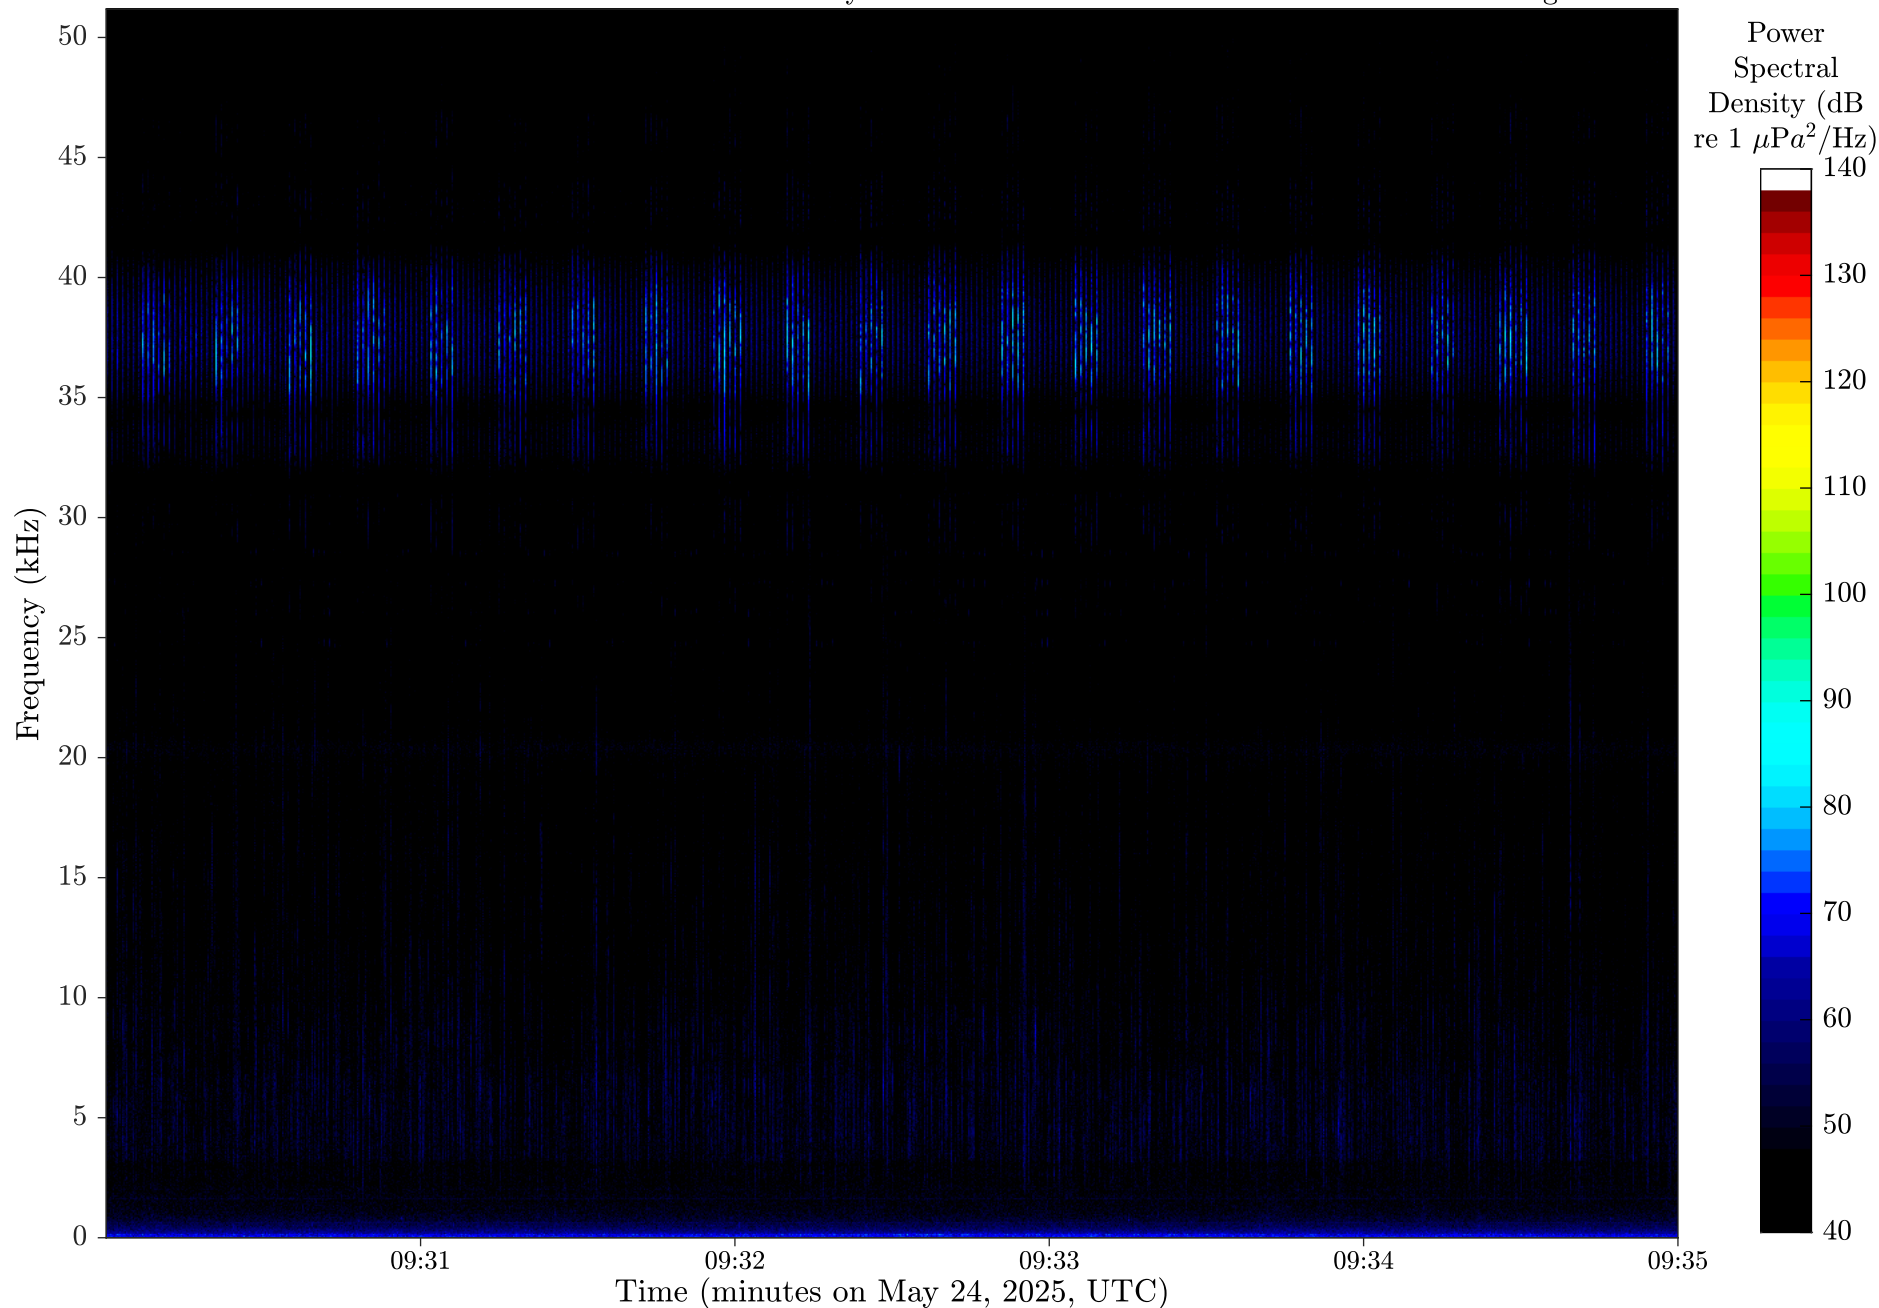

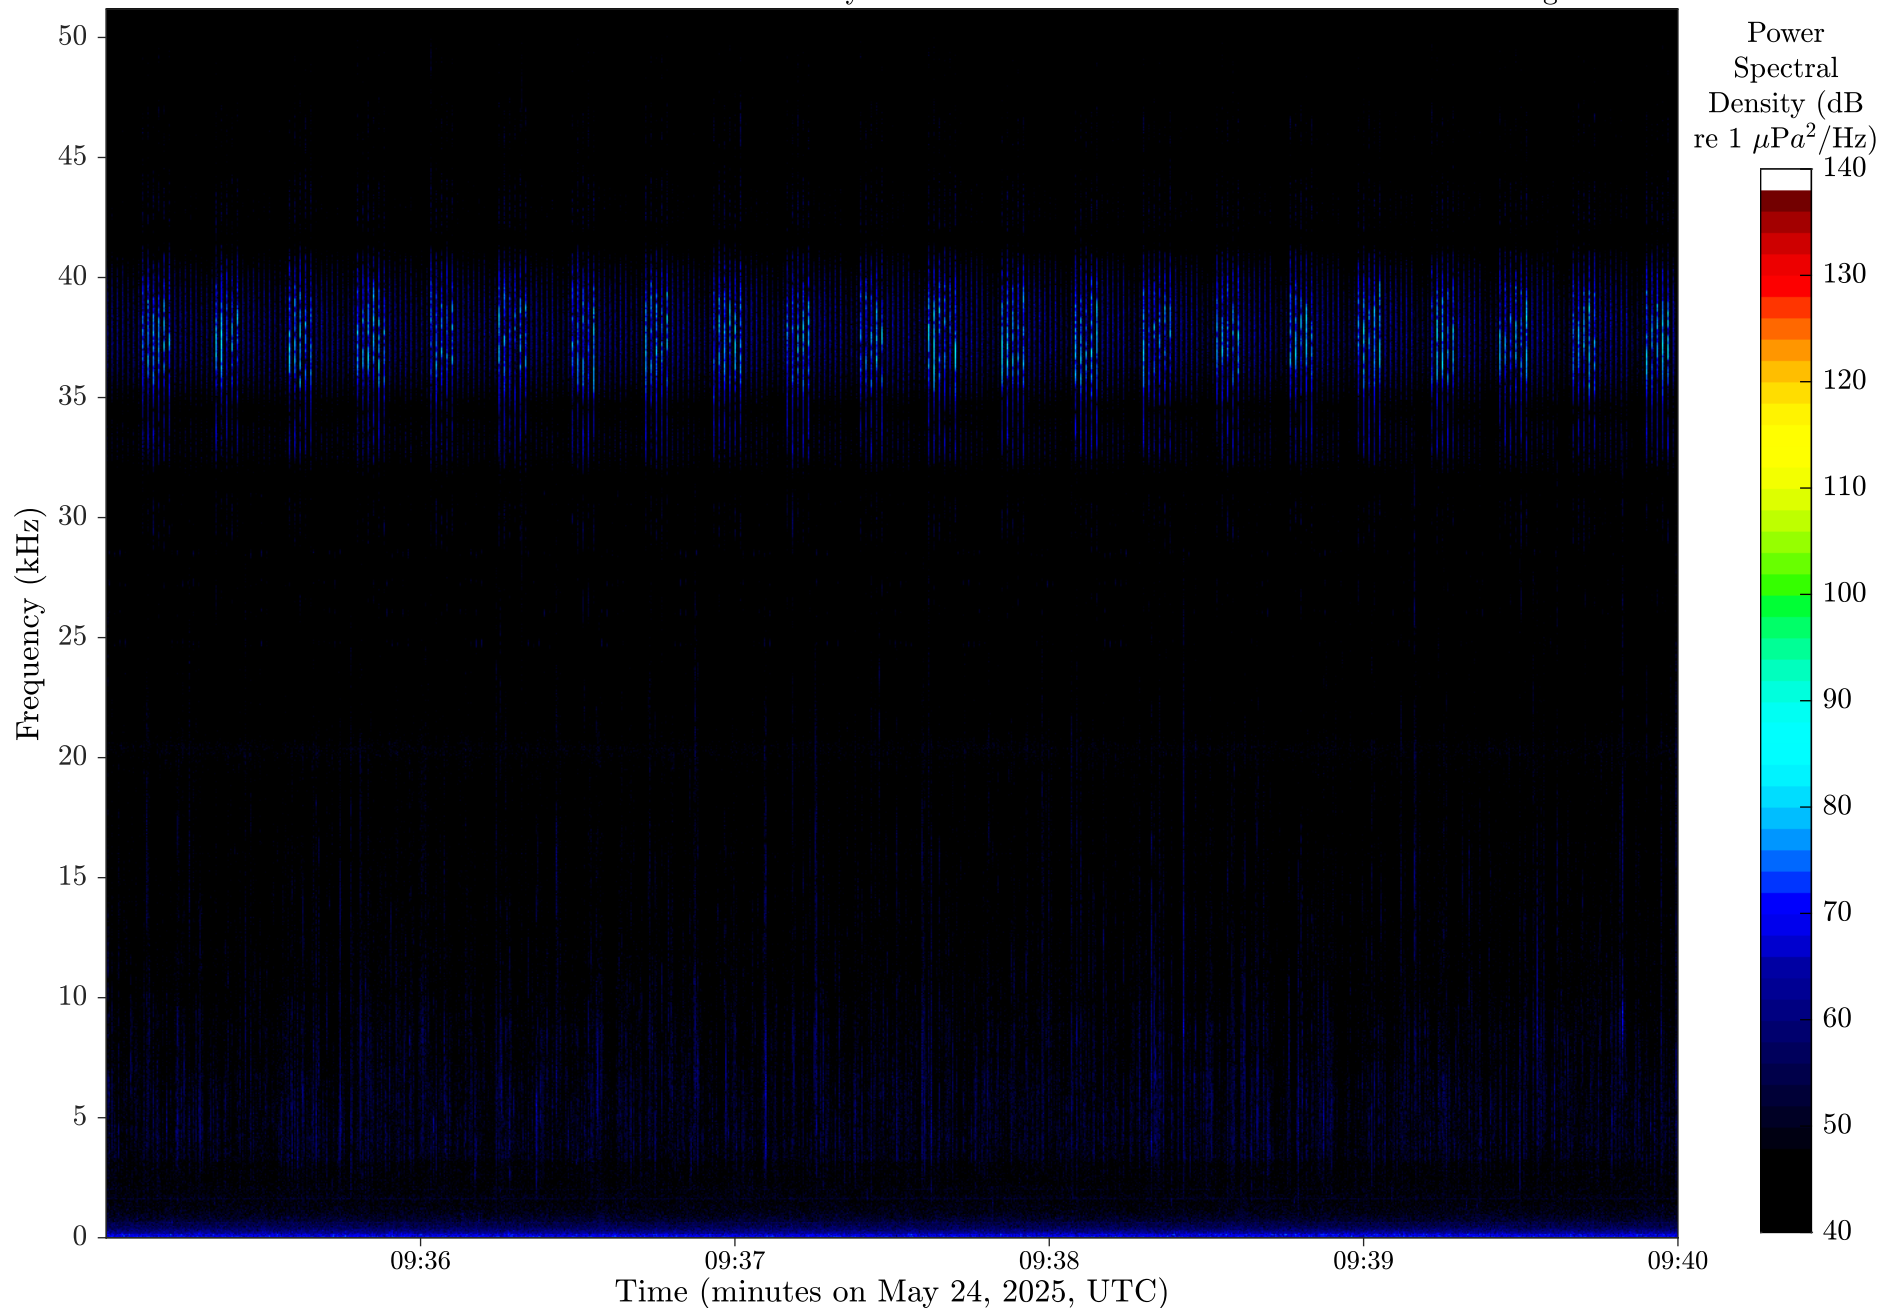


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:26:09 UTC

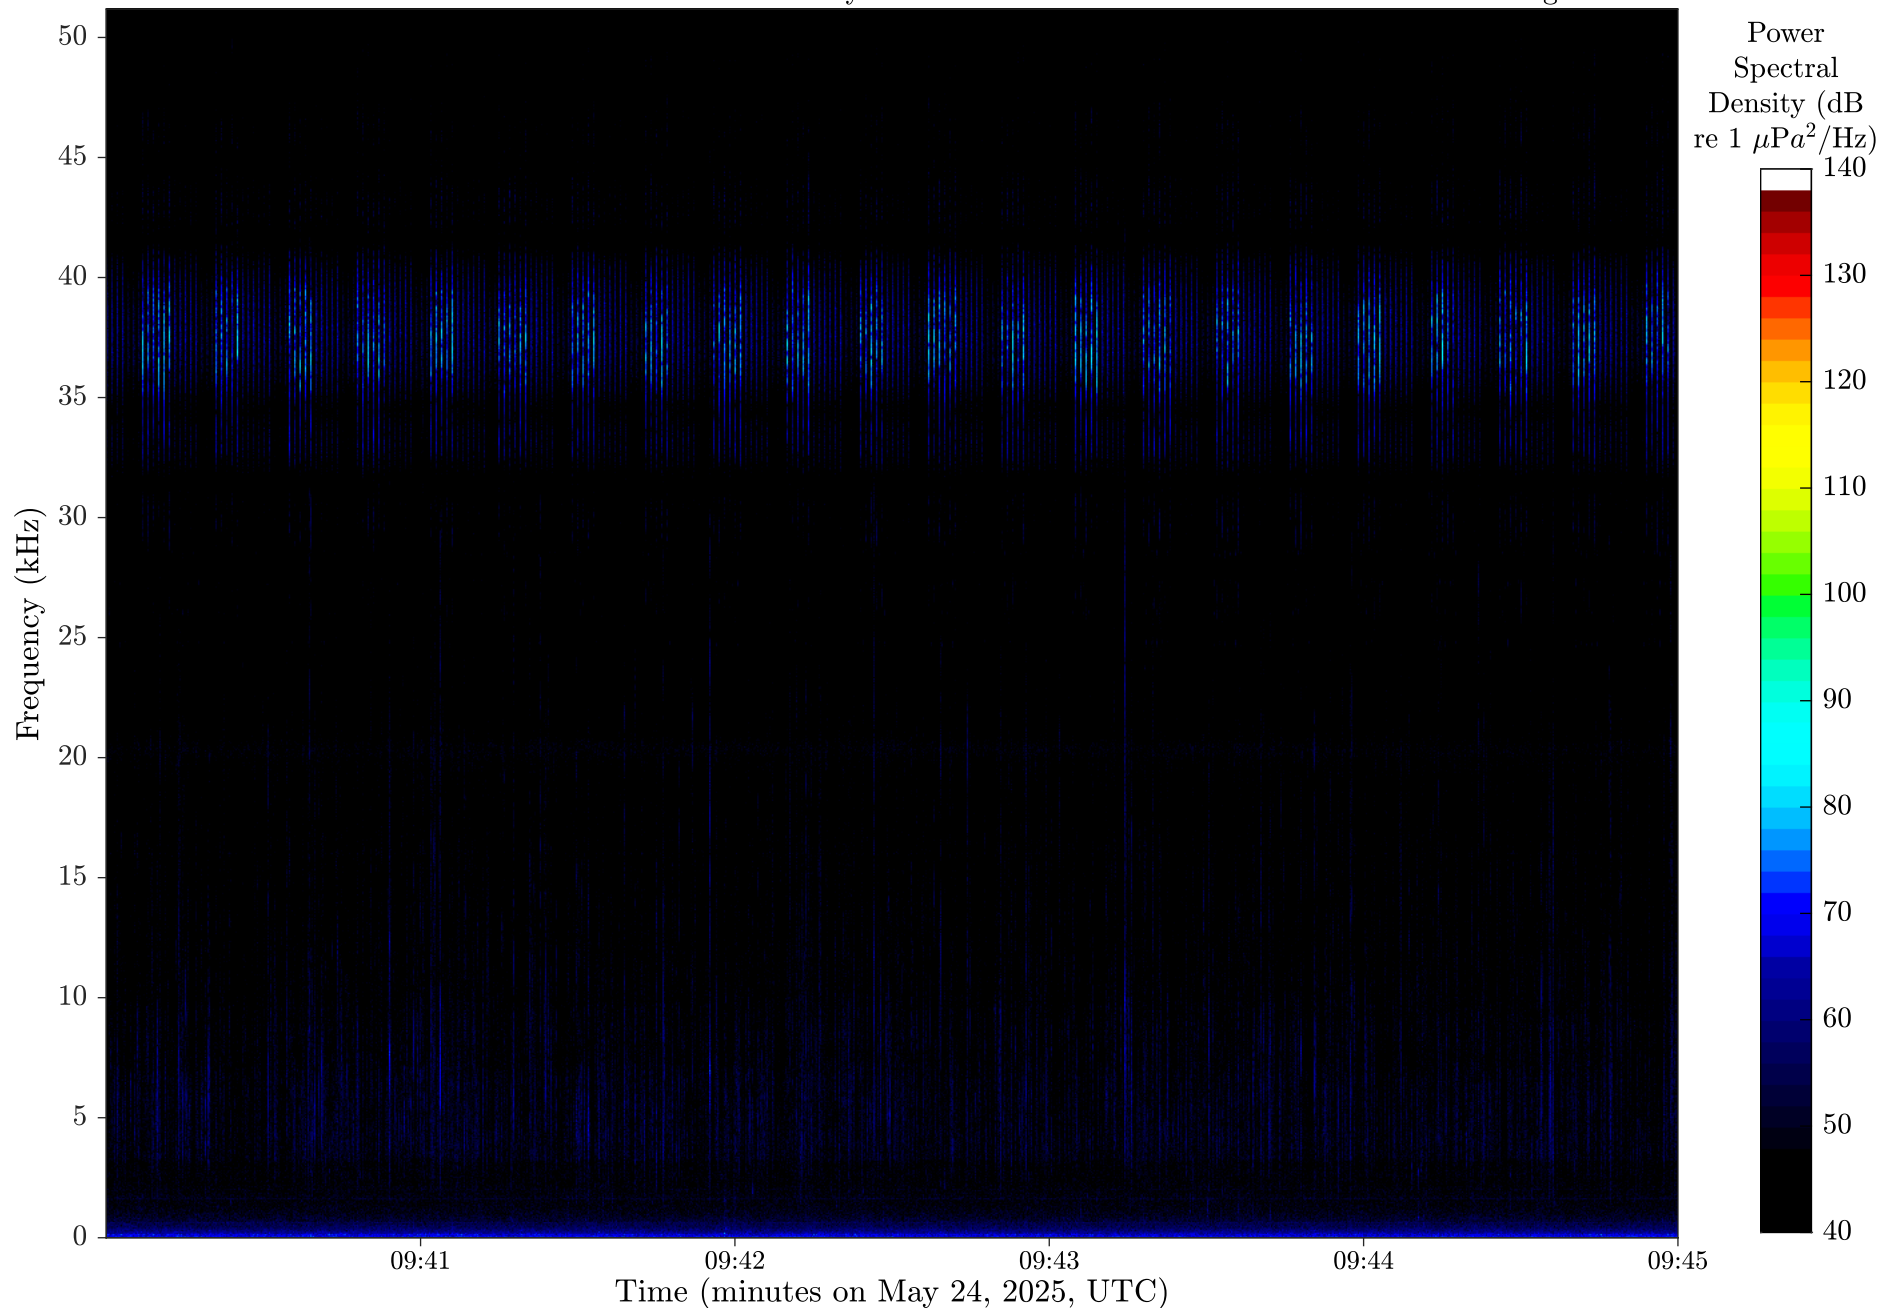


Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:26:17 UTC

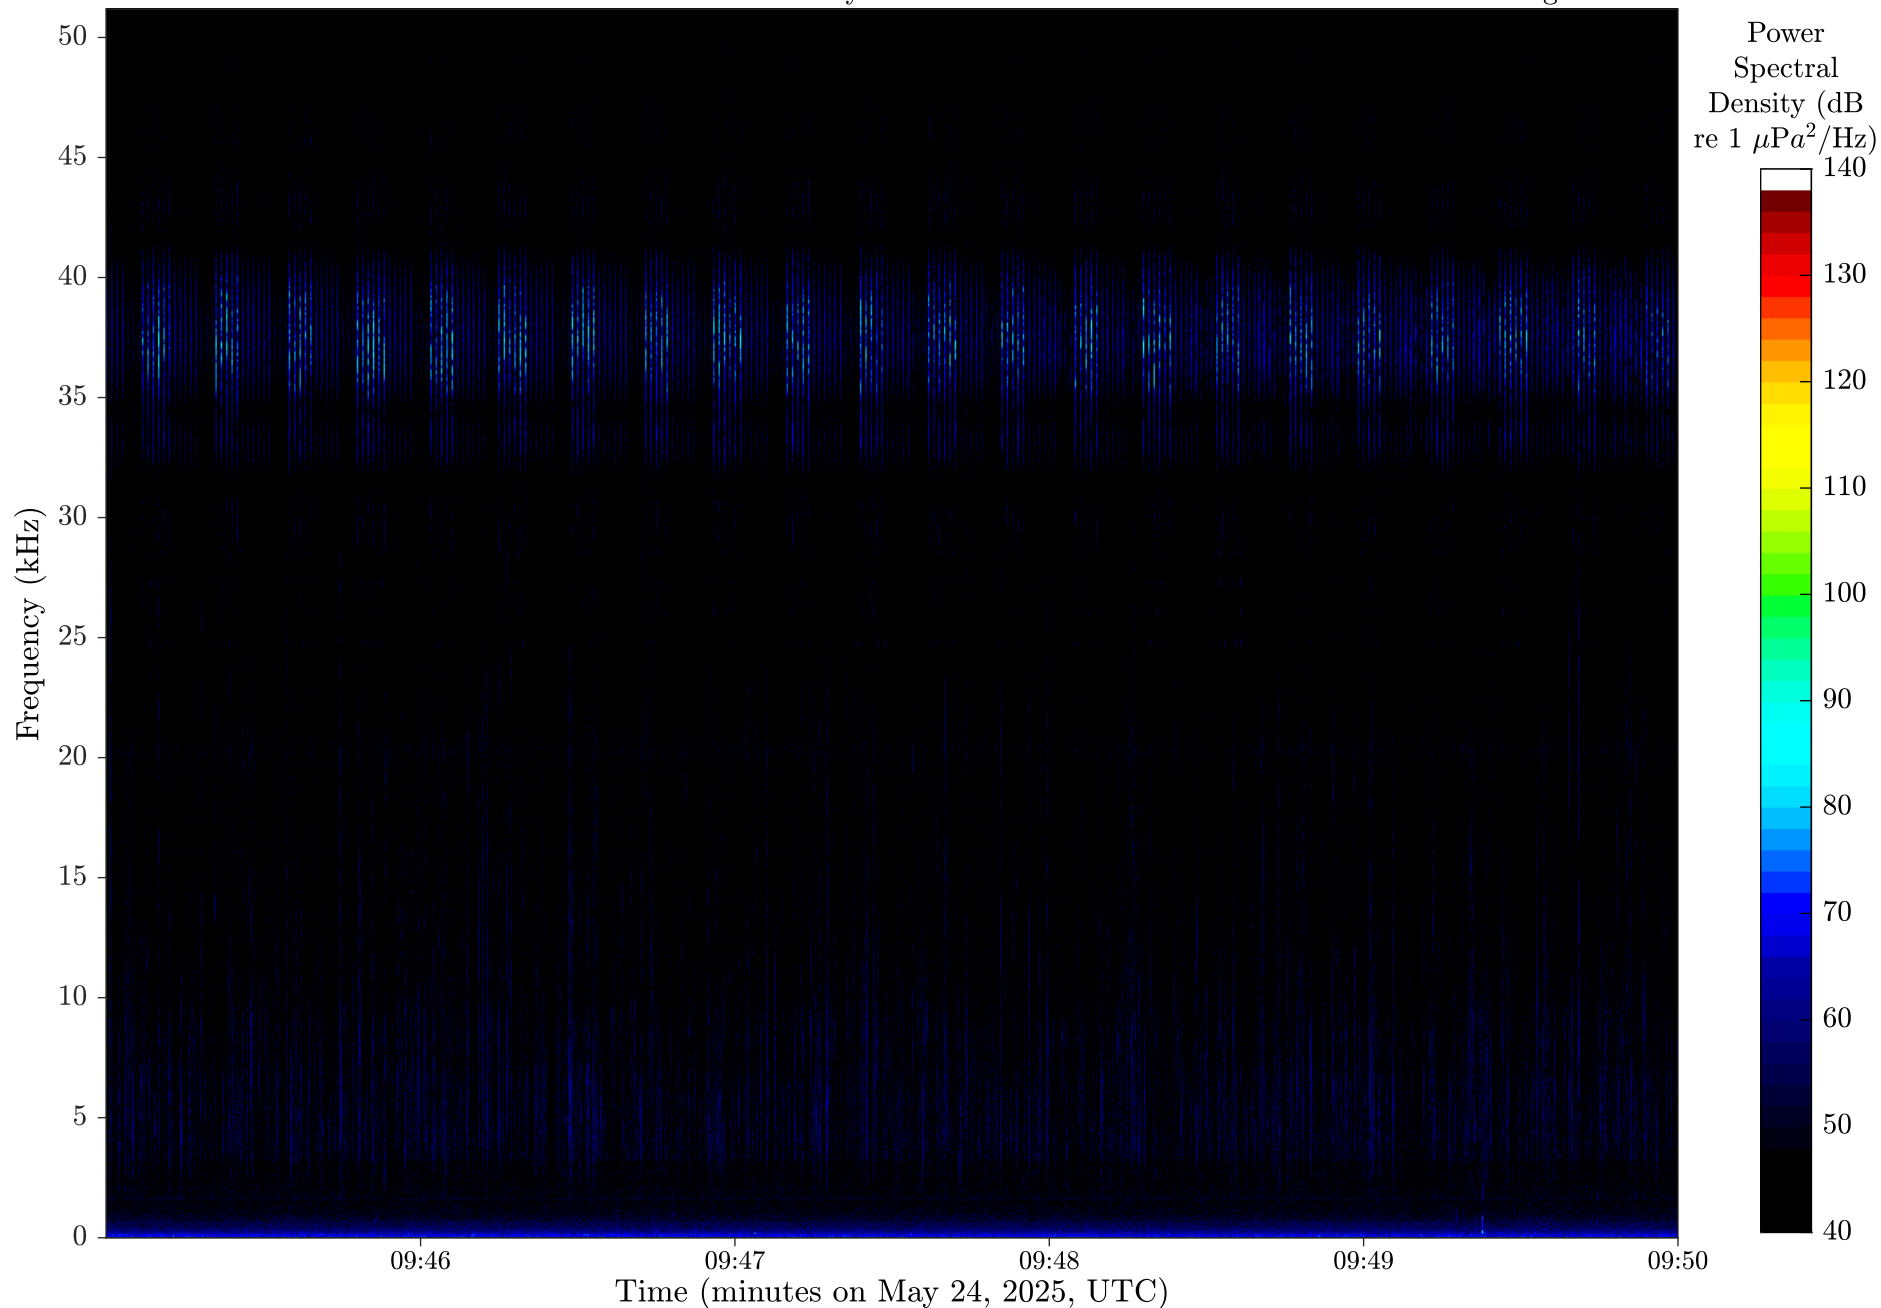


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:26:24 UTC

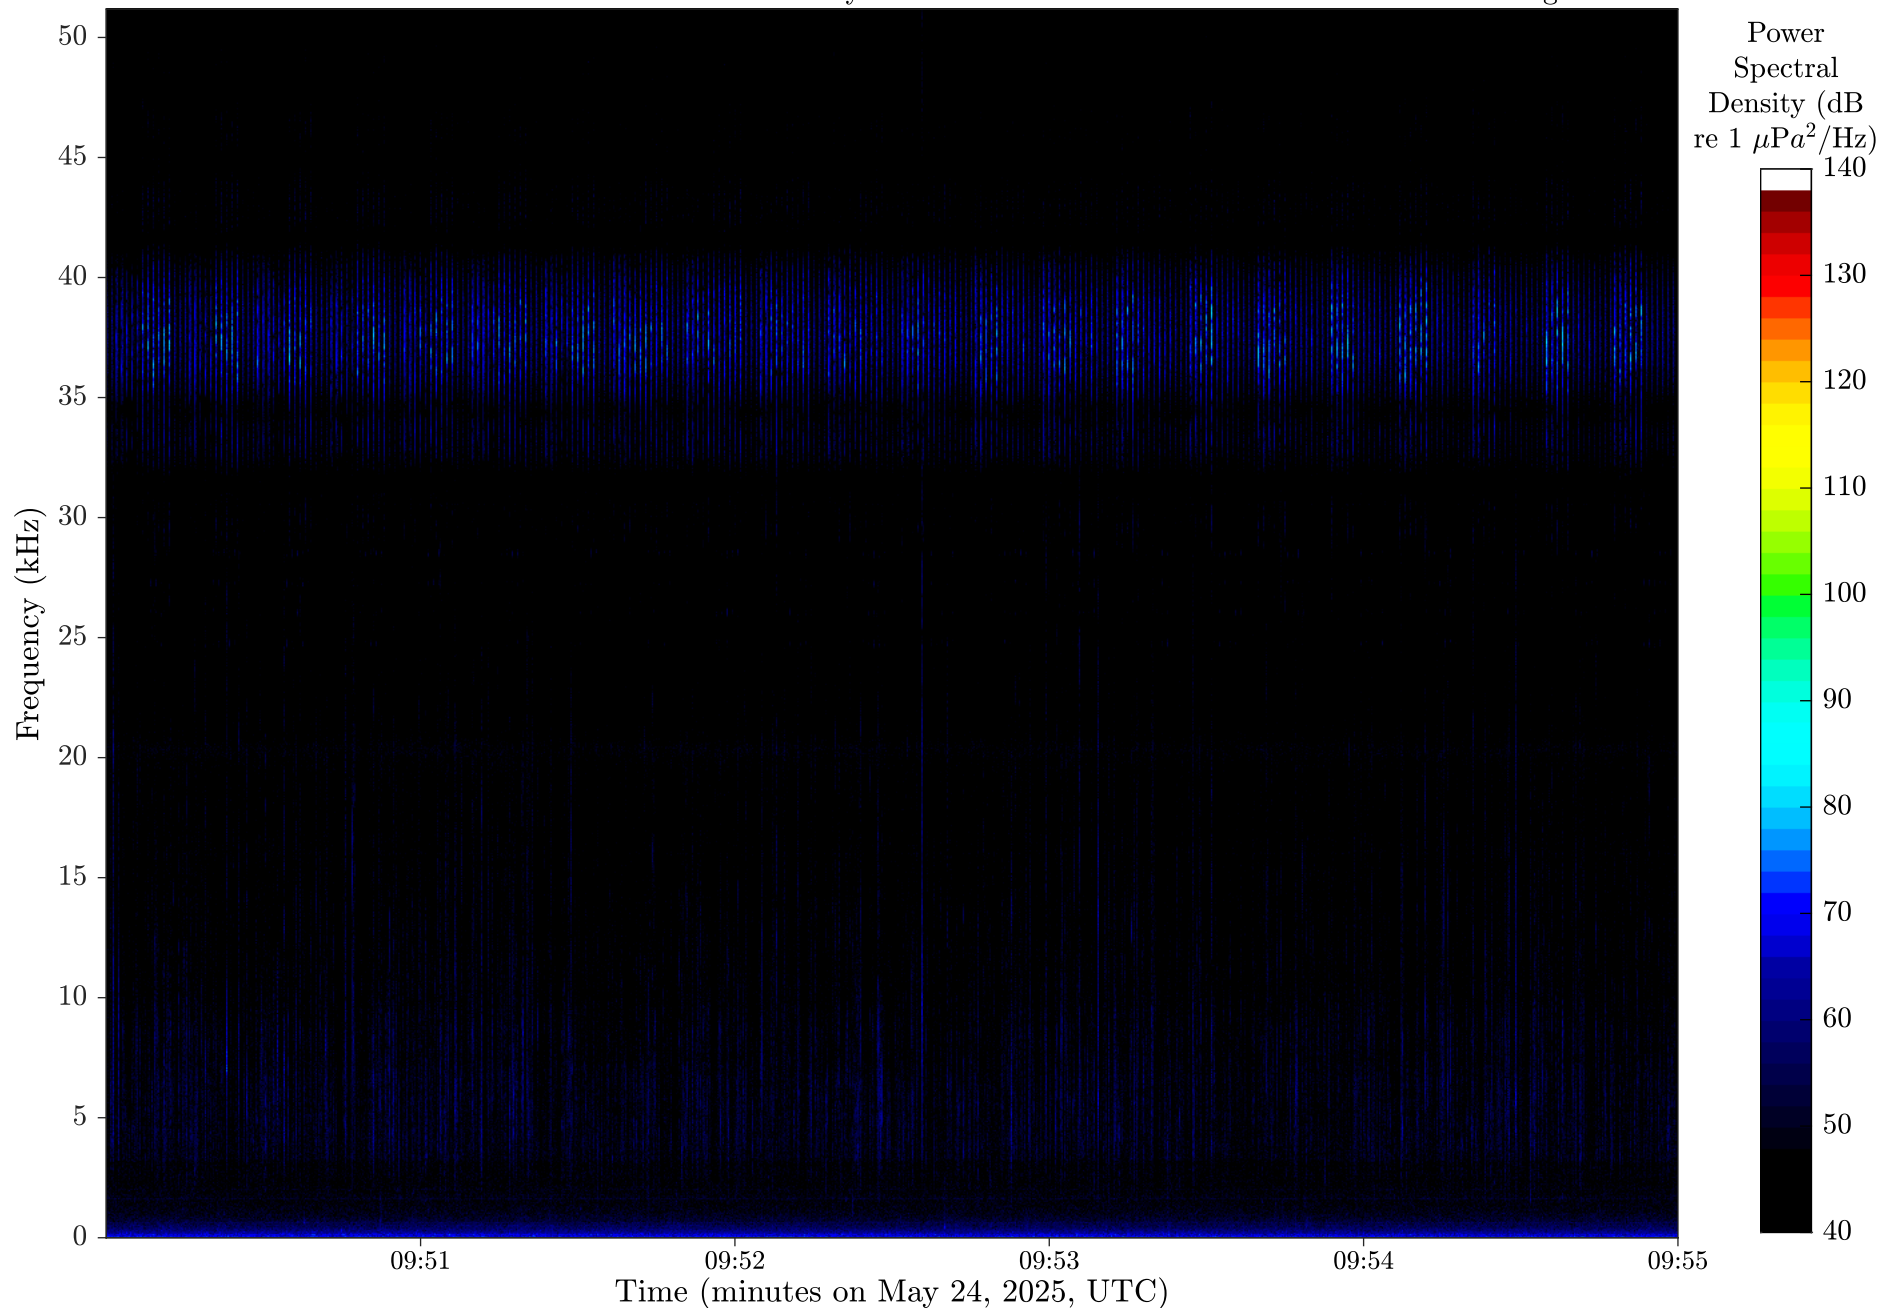


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:26:31 UTC

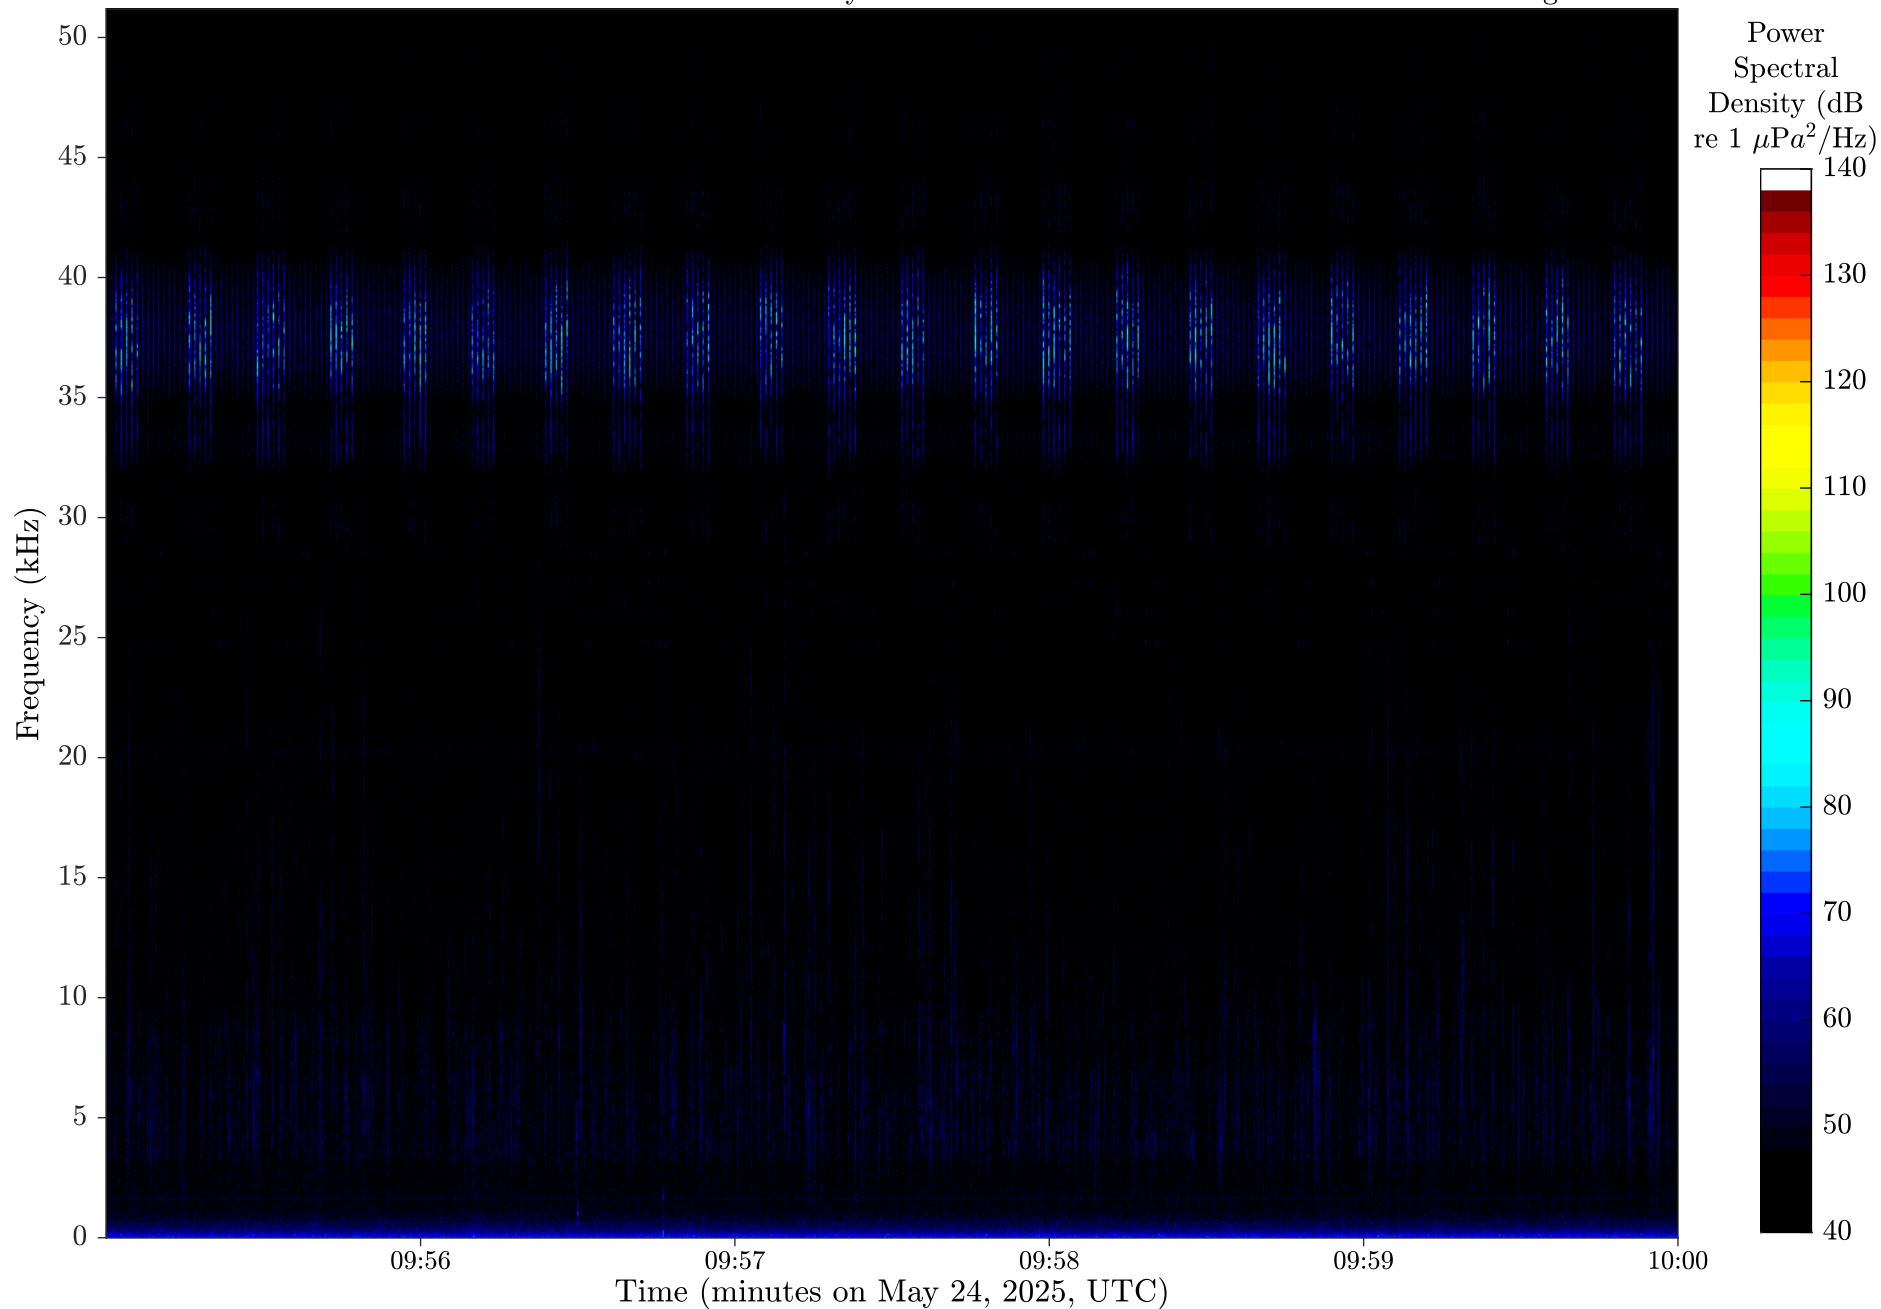


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:26:38 UTC

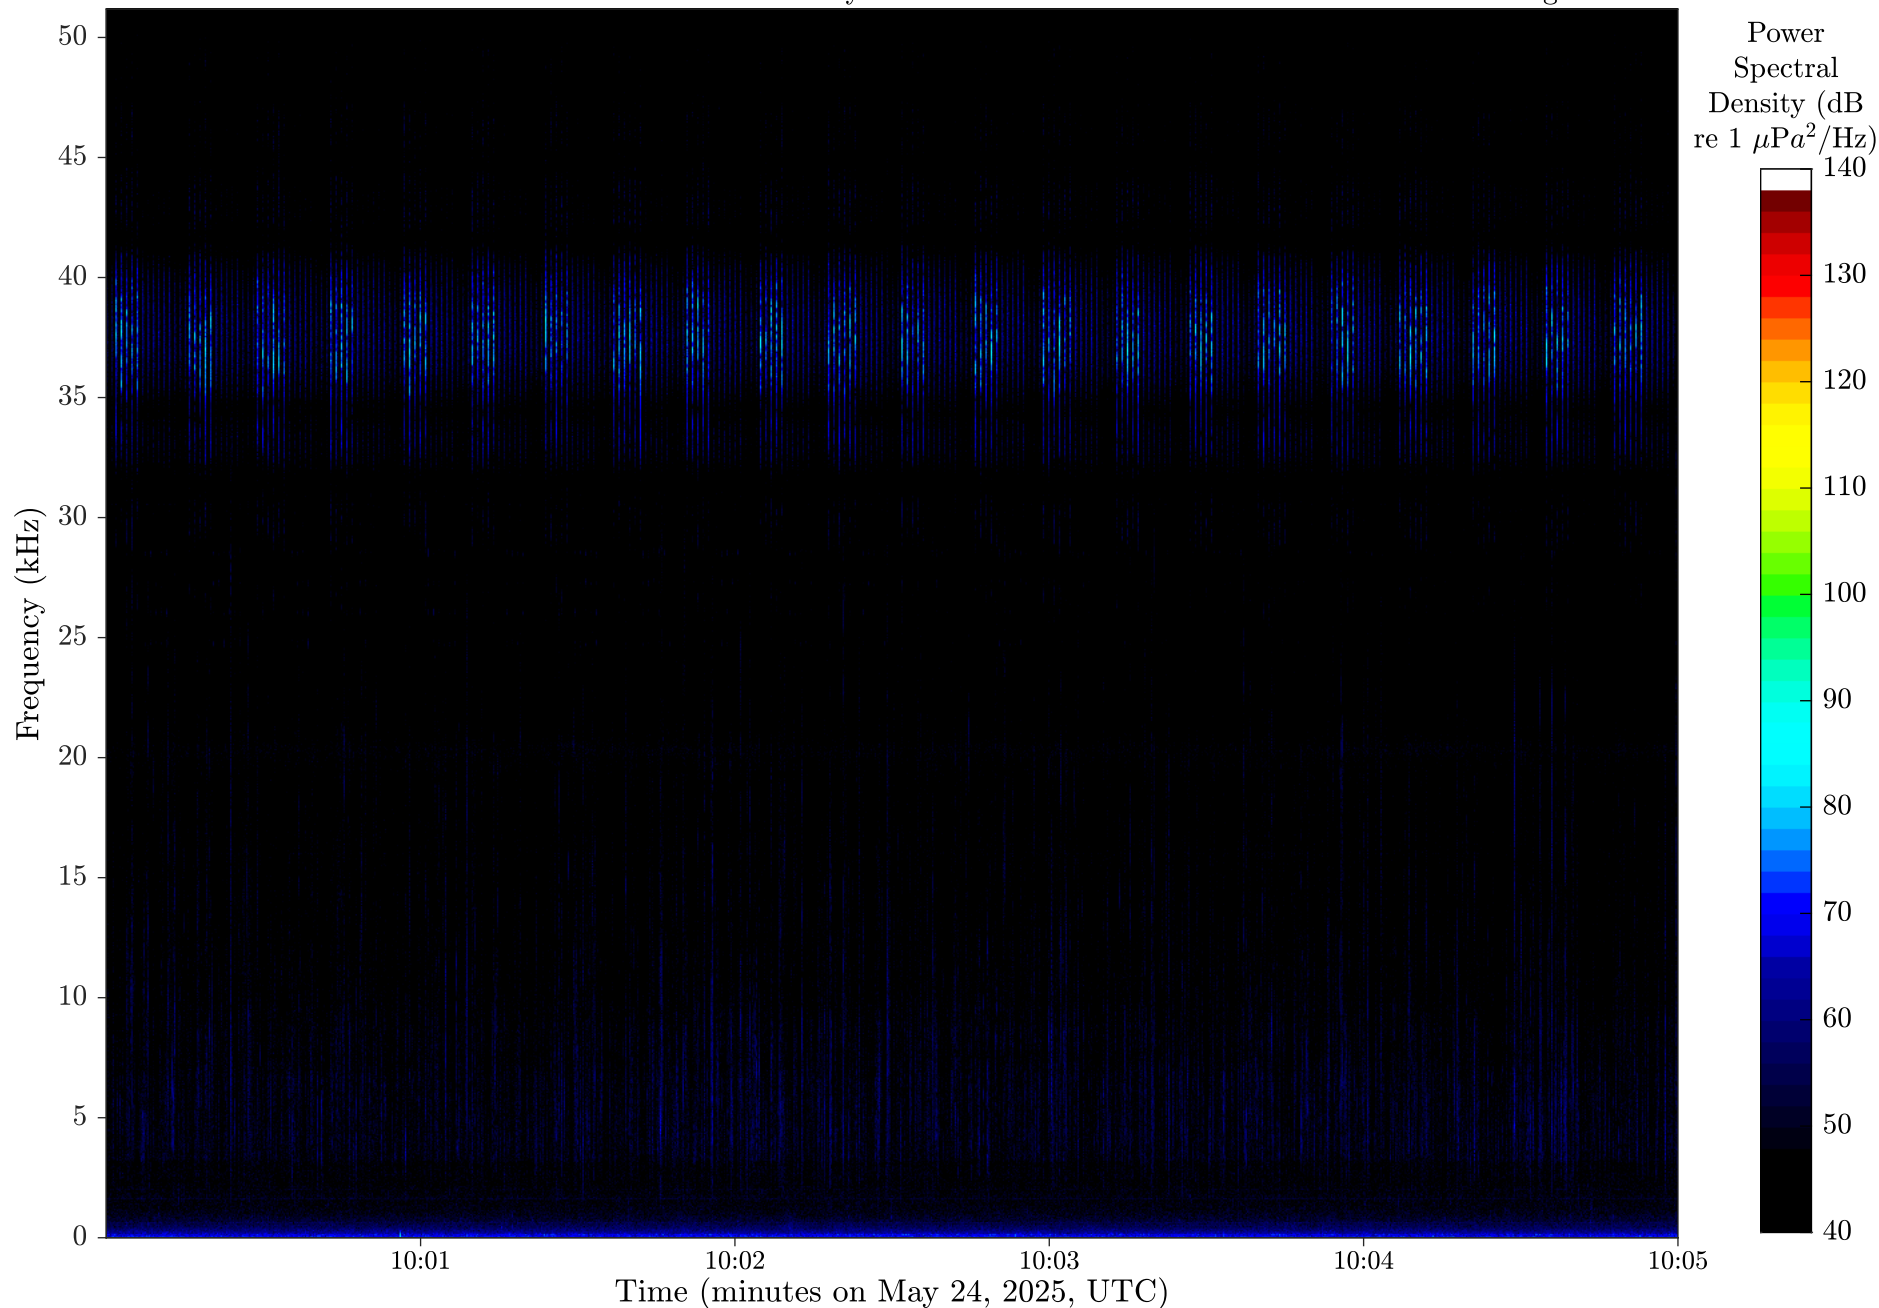


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:26:46 UTC

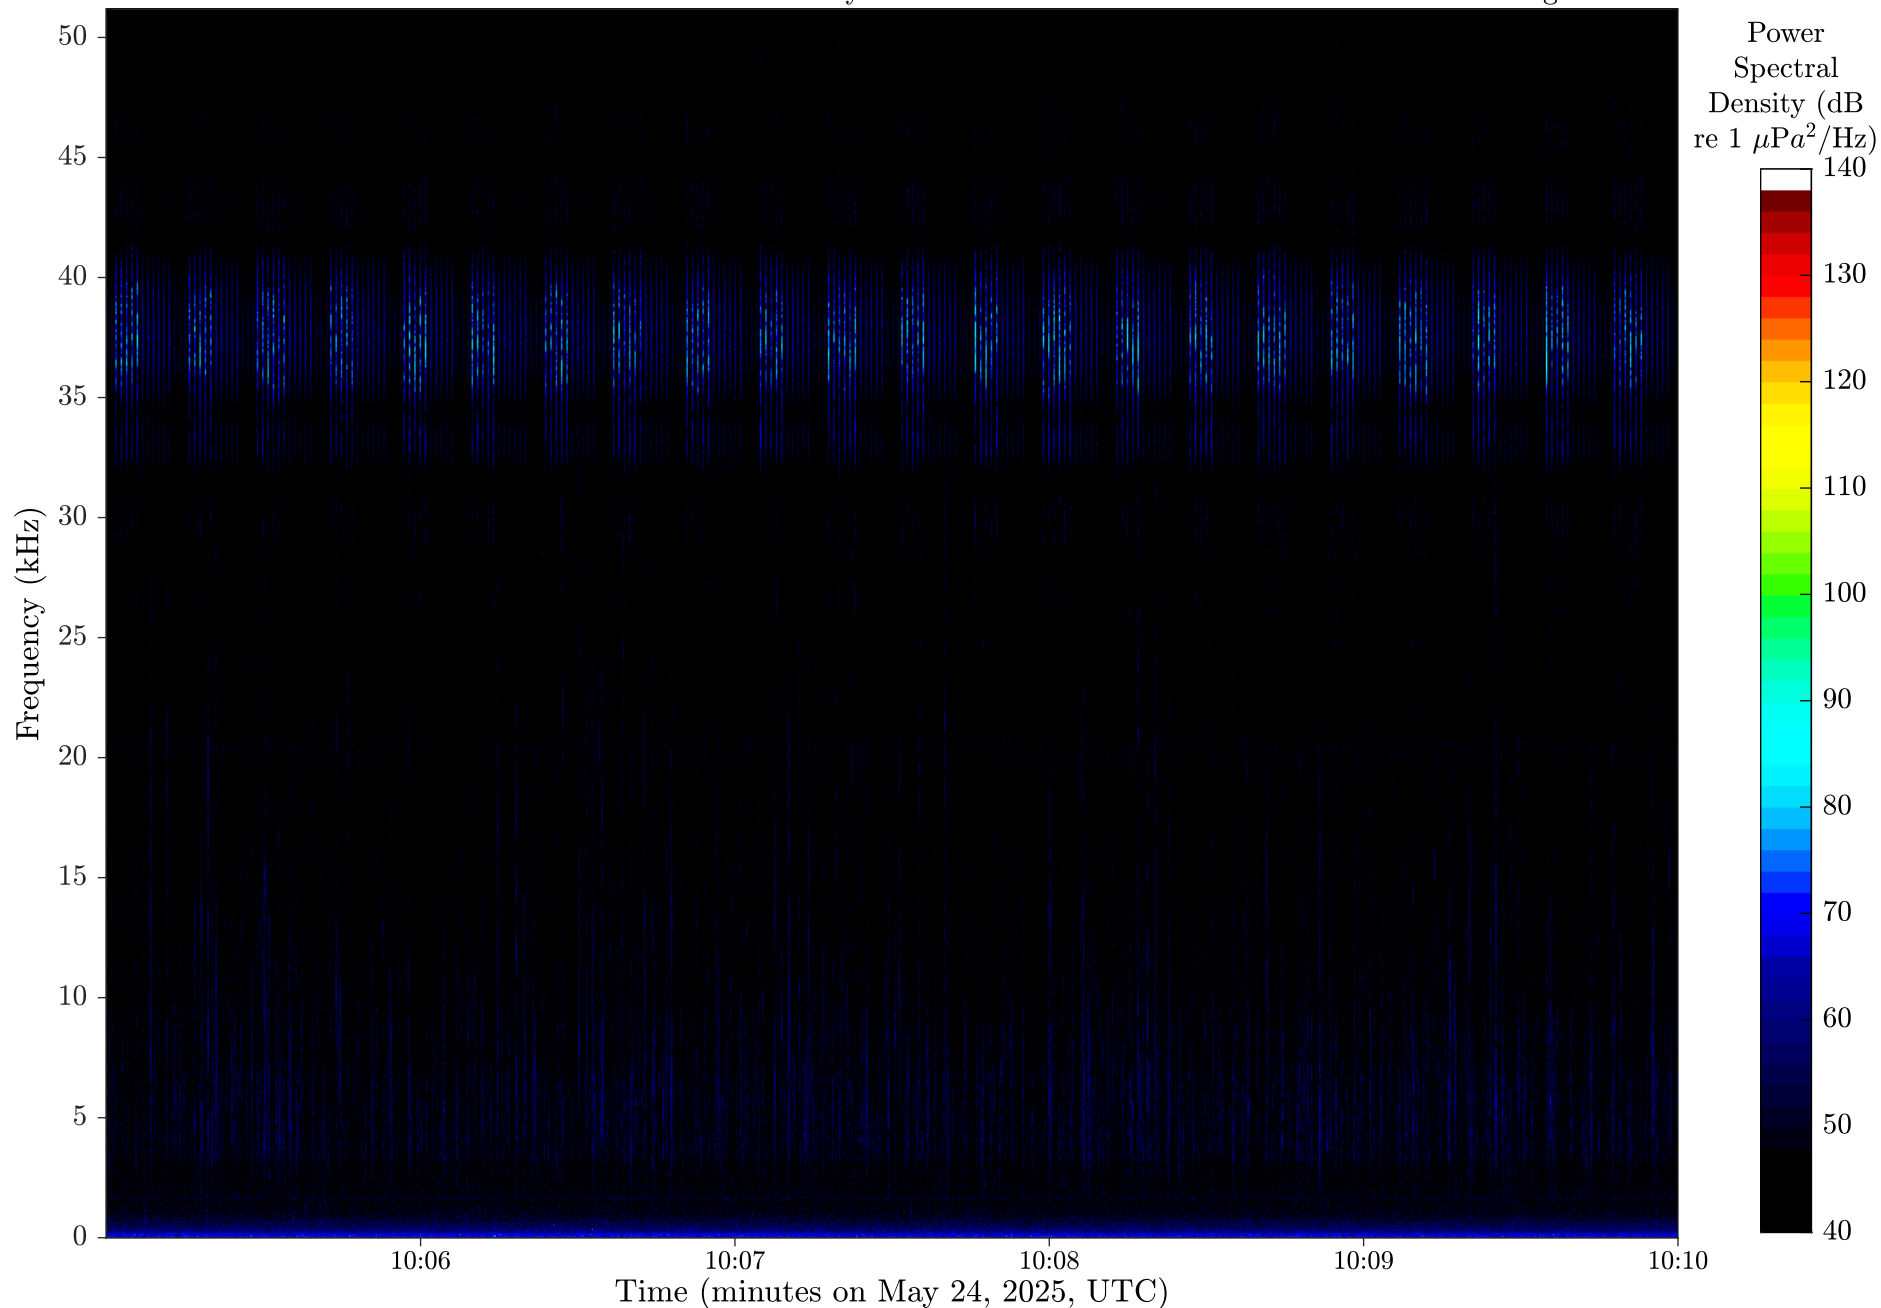



Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:26:53 UTC

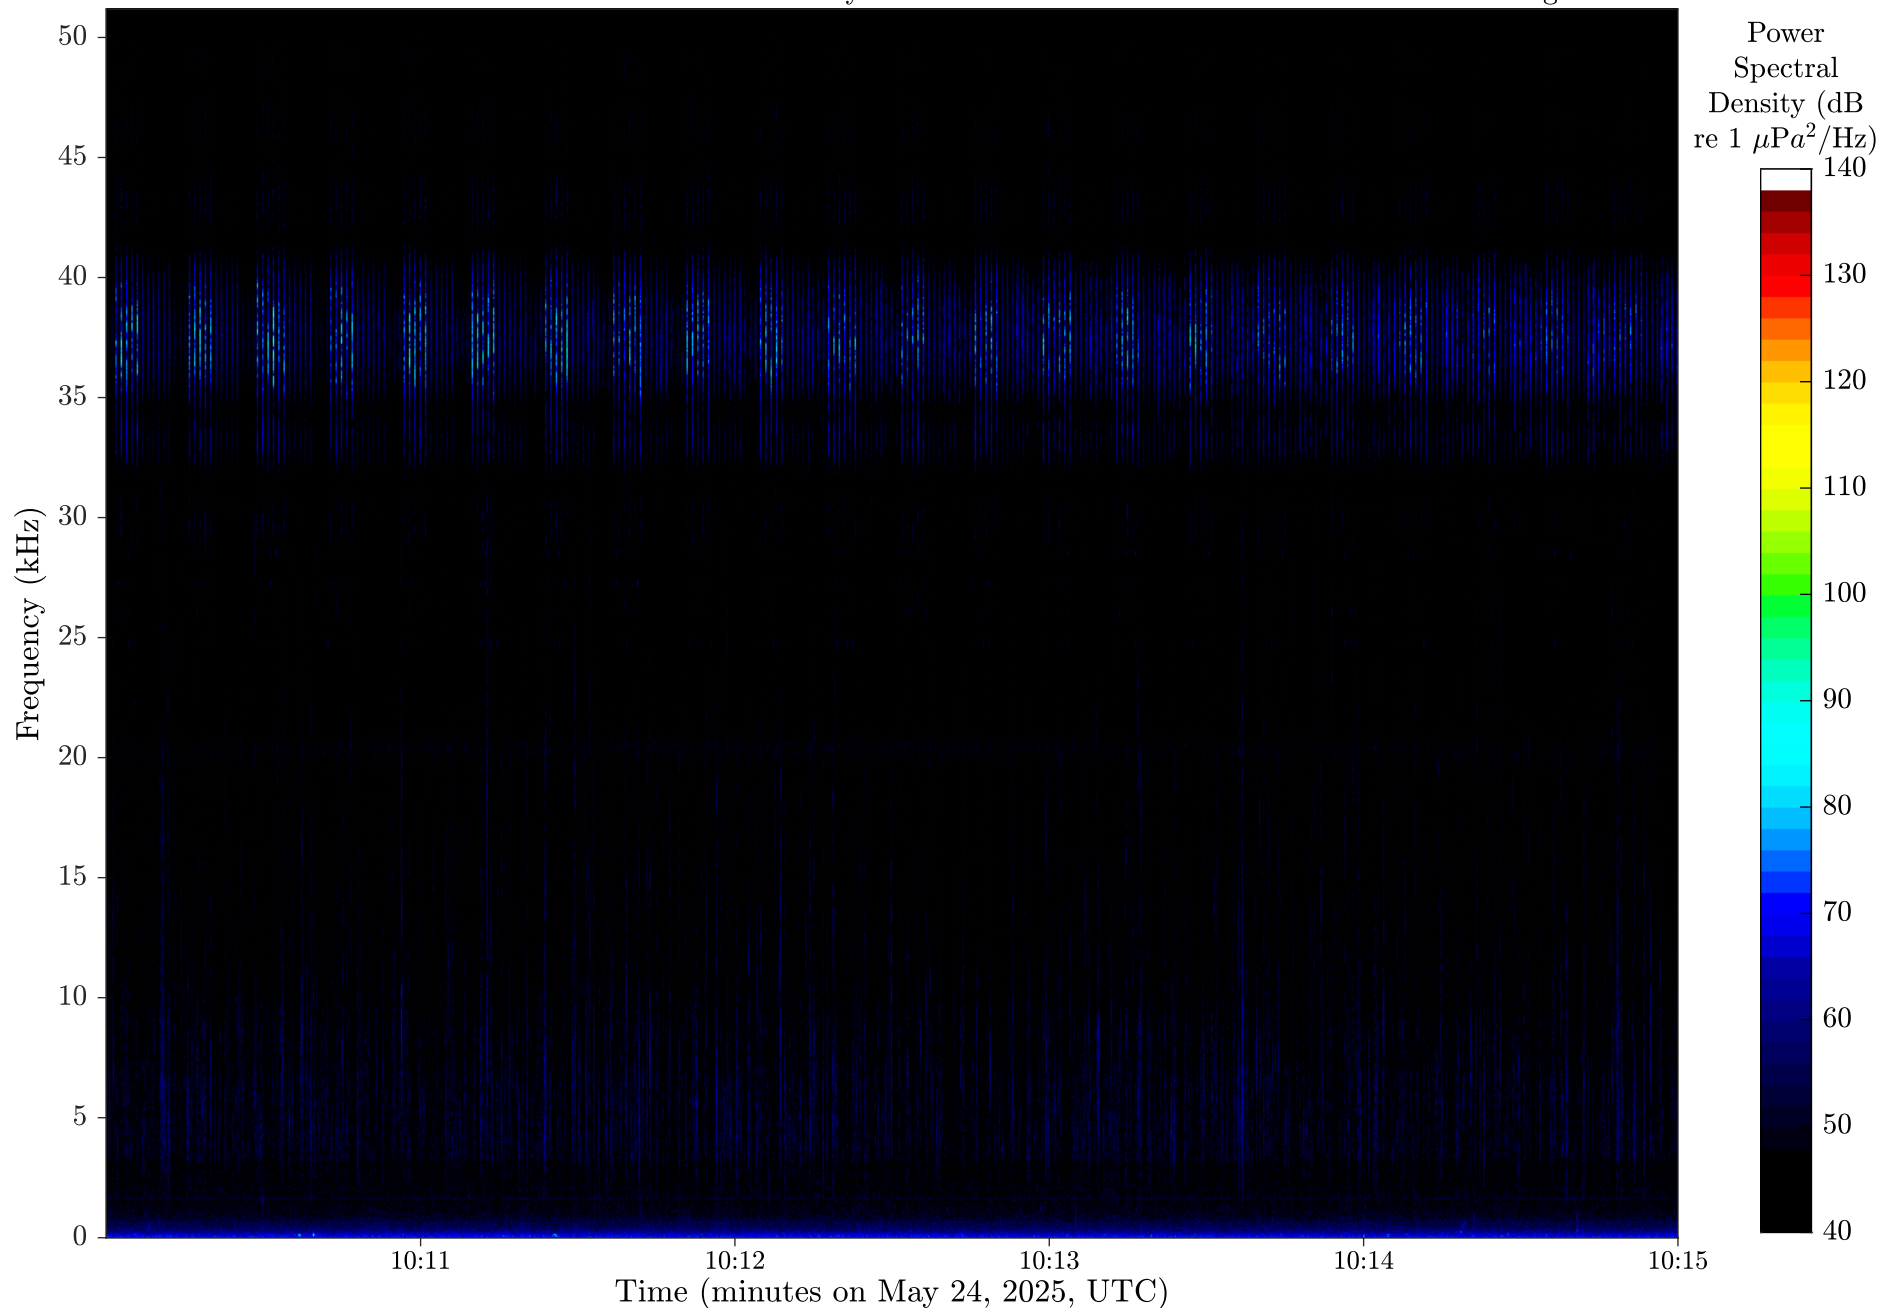

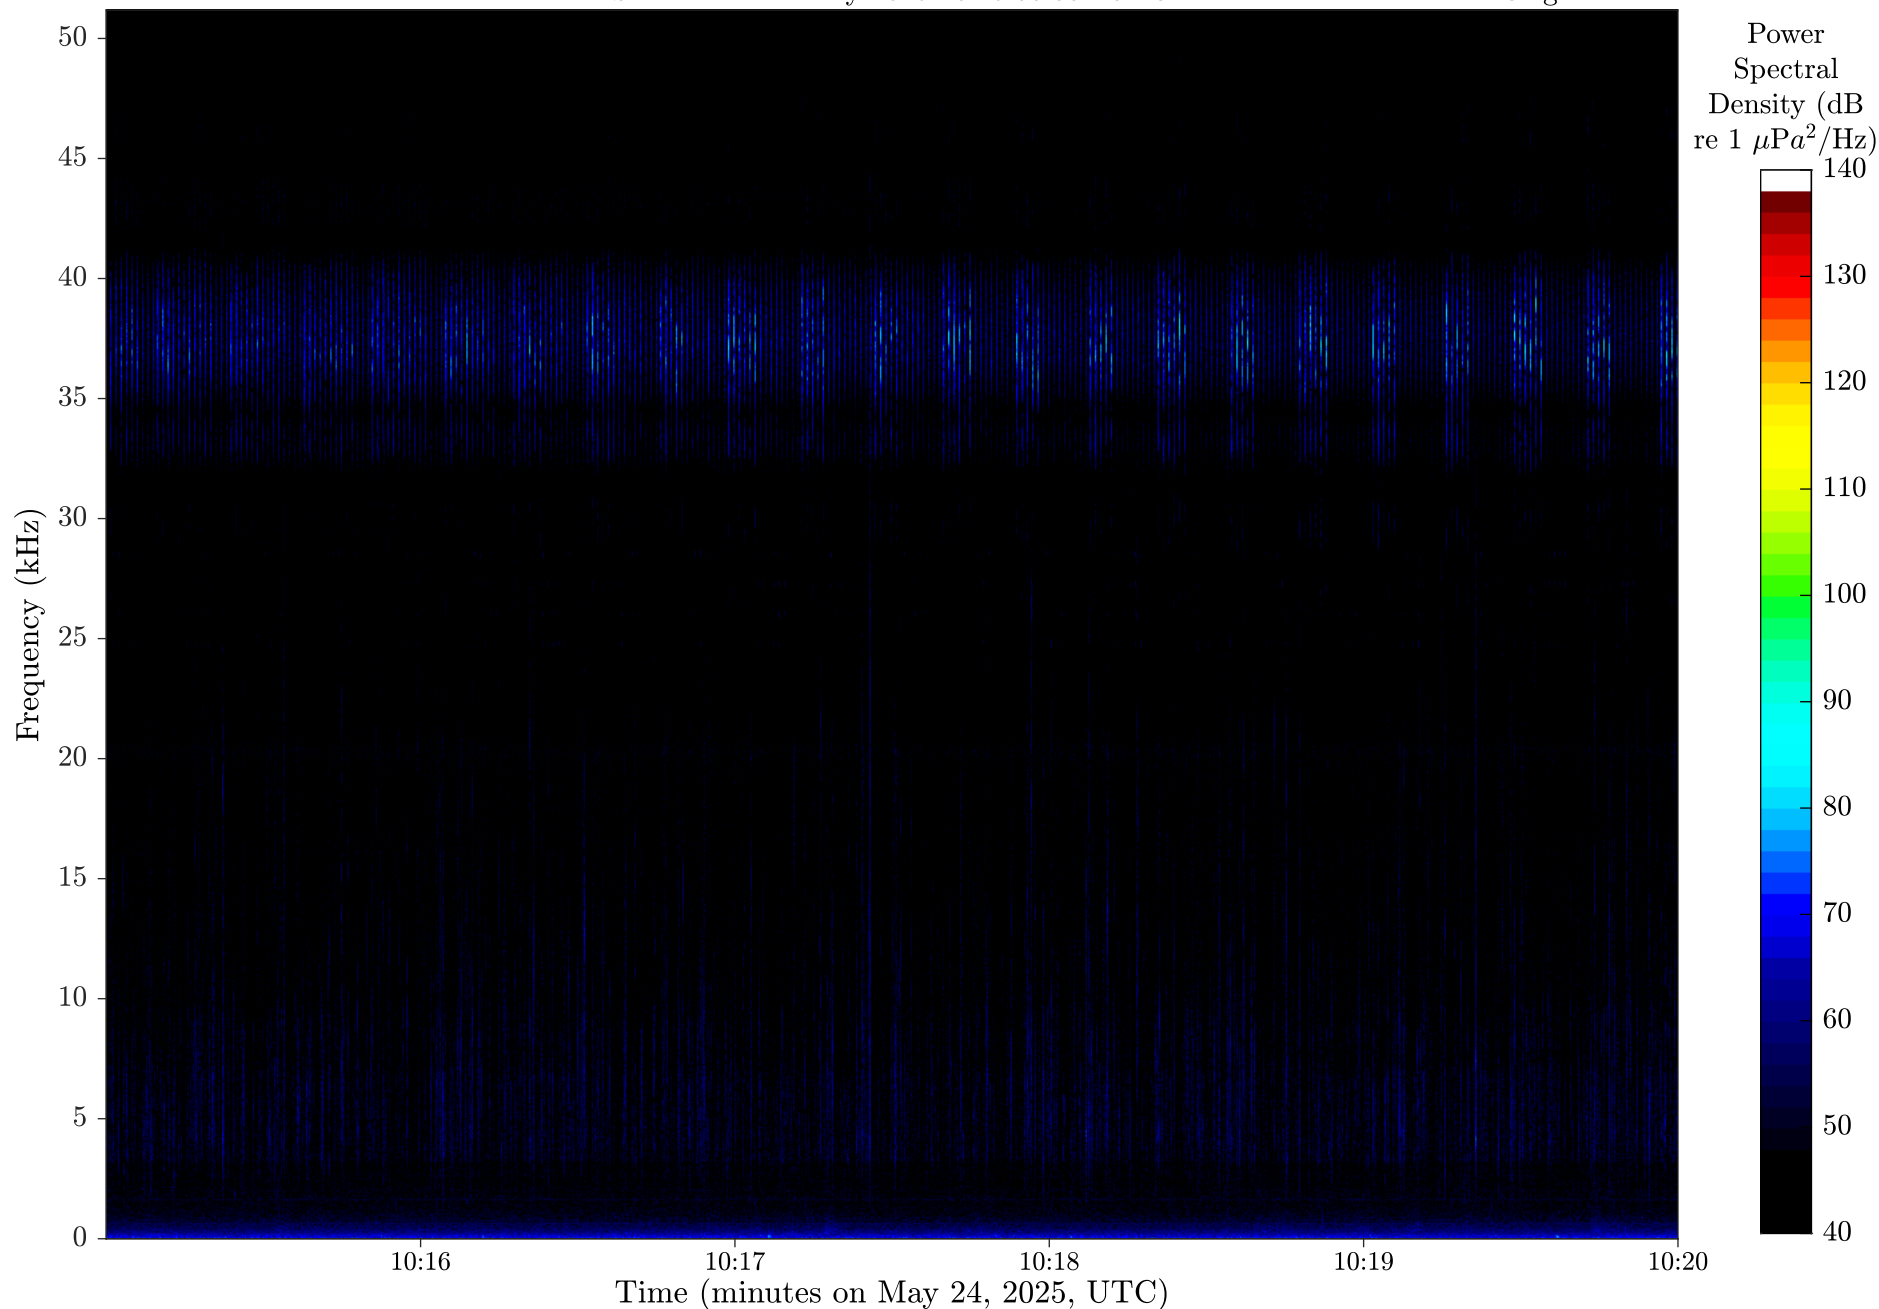


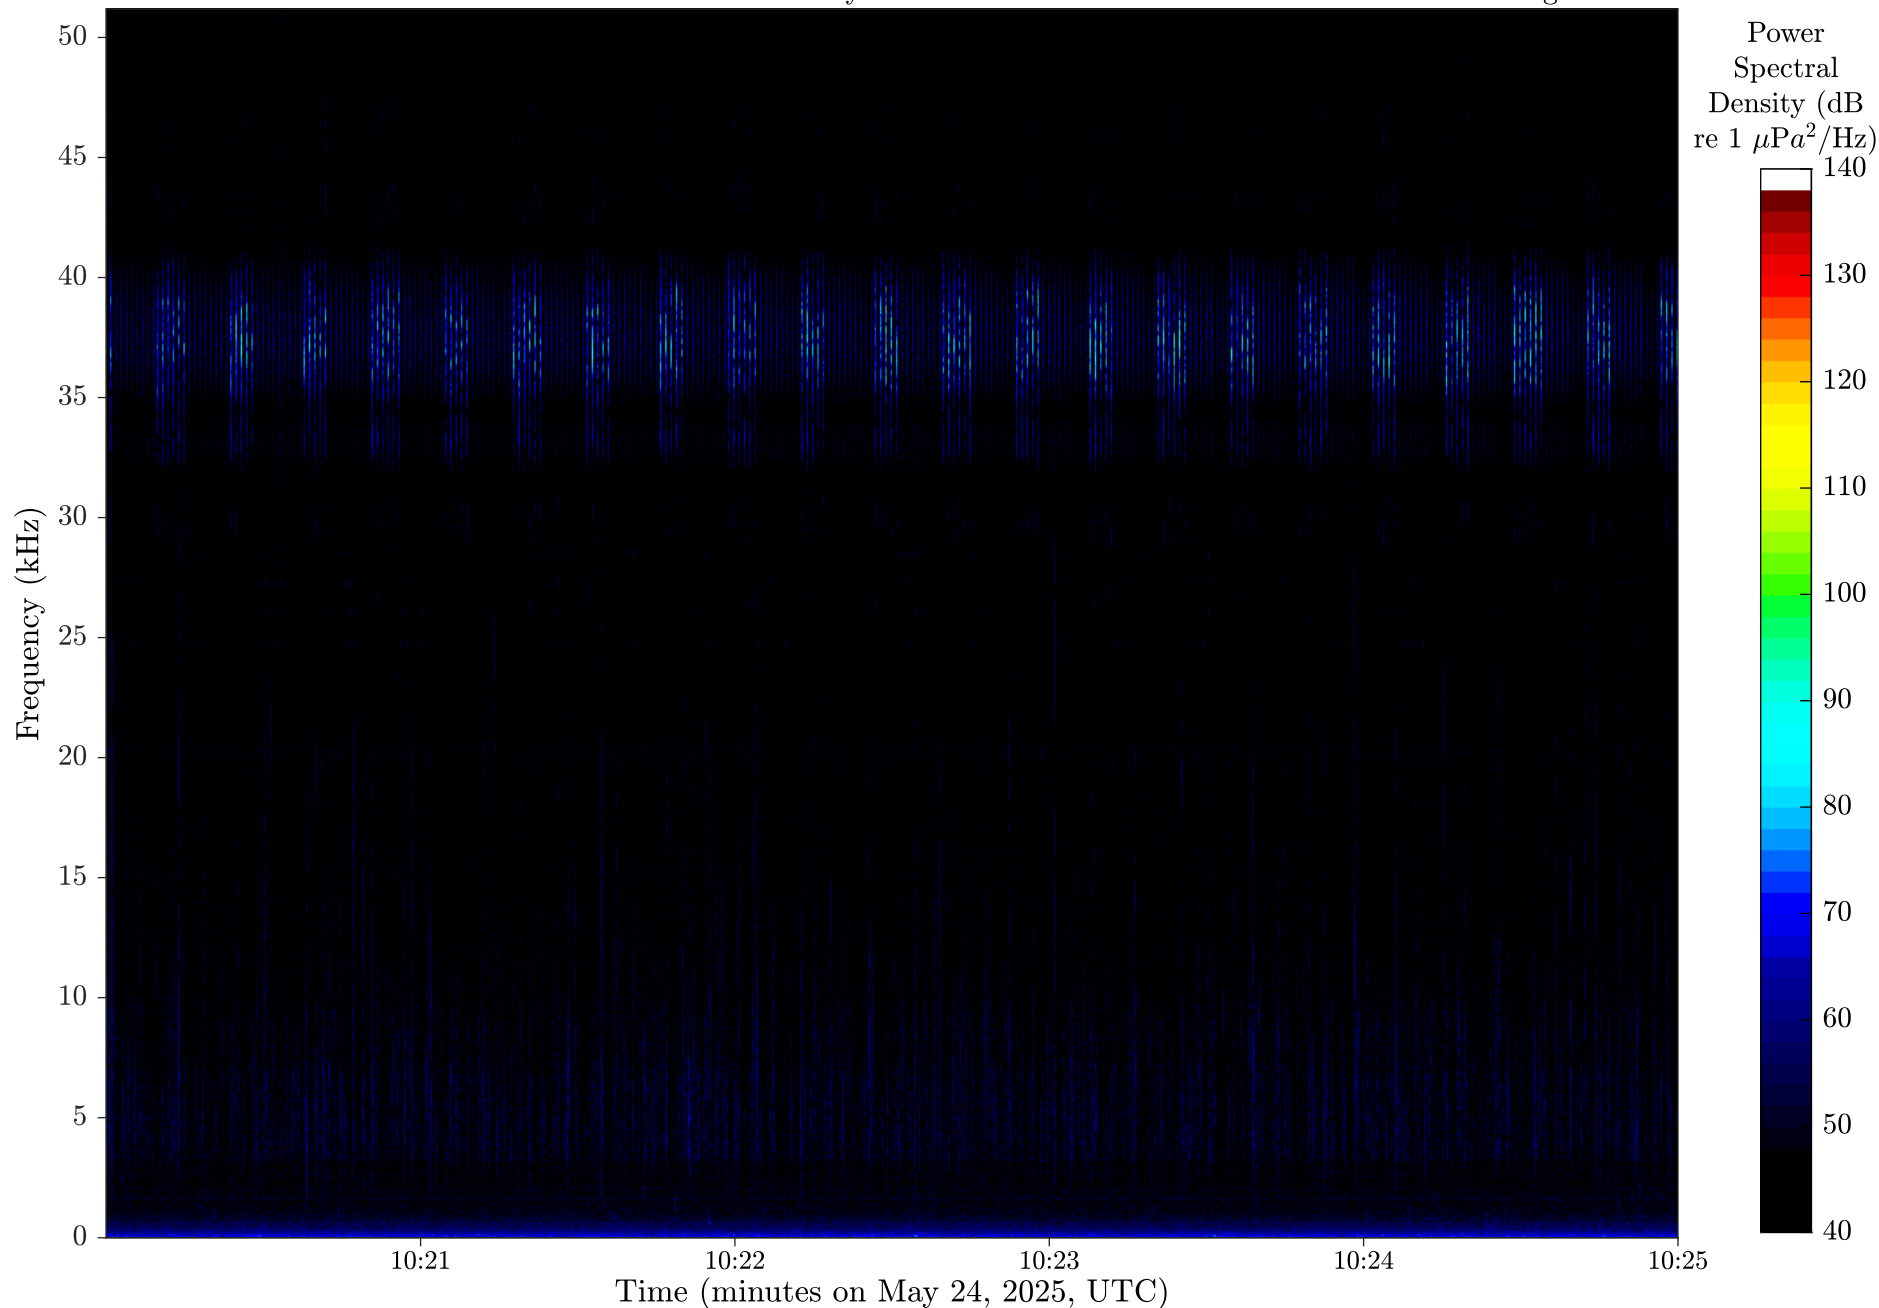


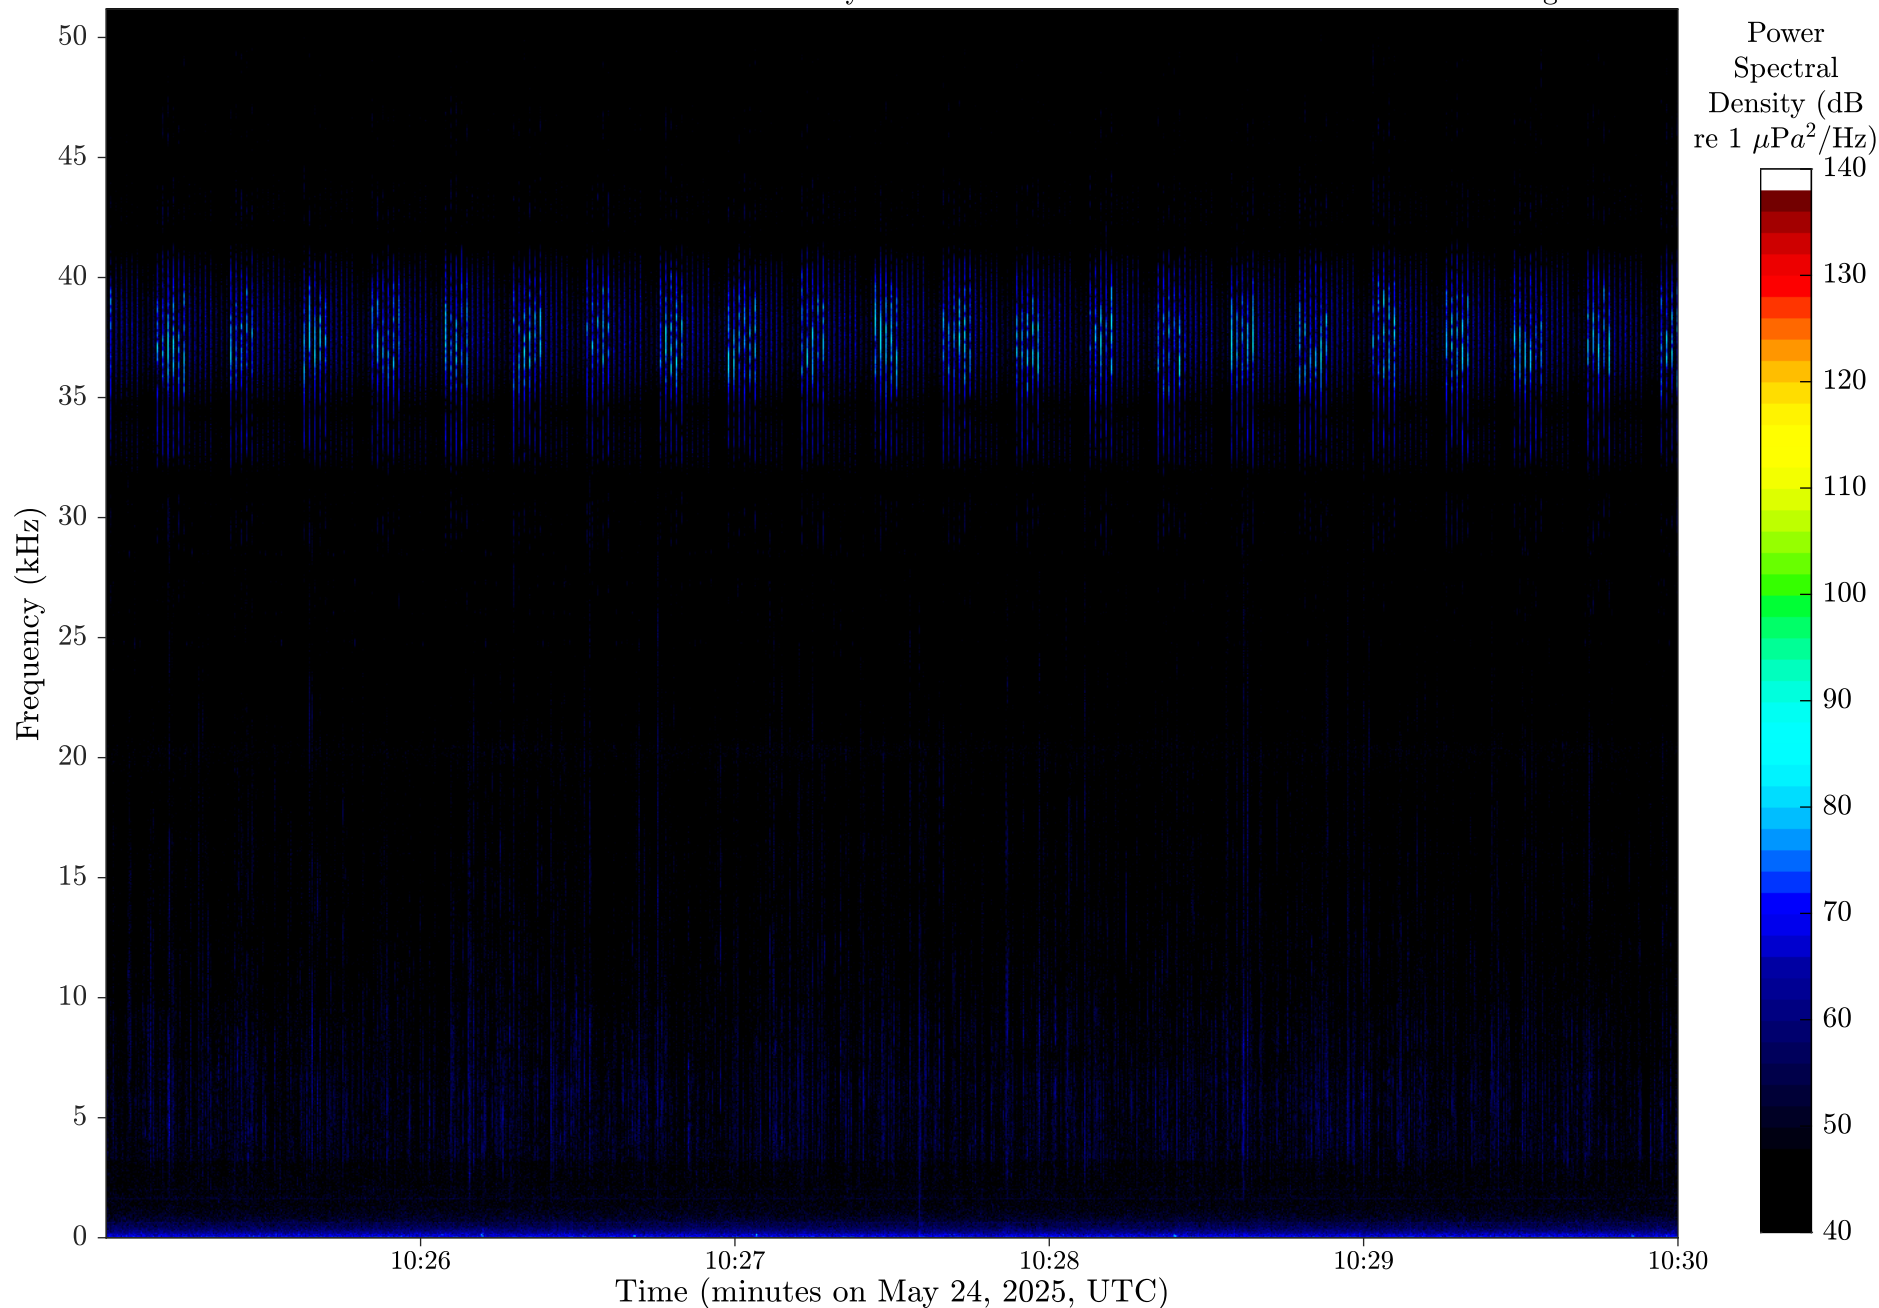

Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:27:23 UTC

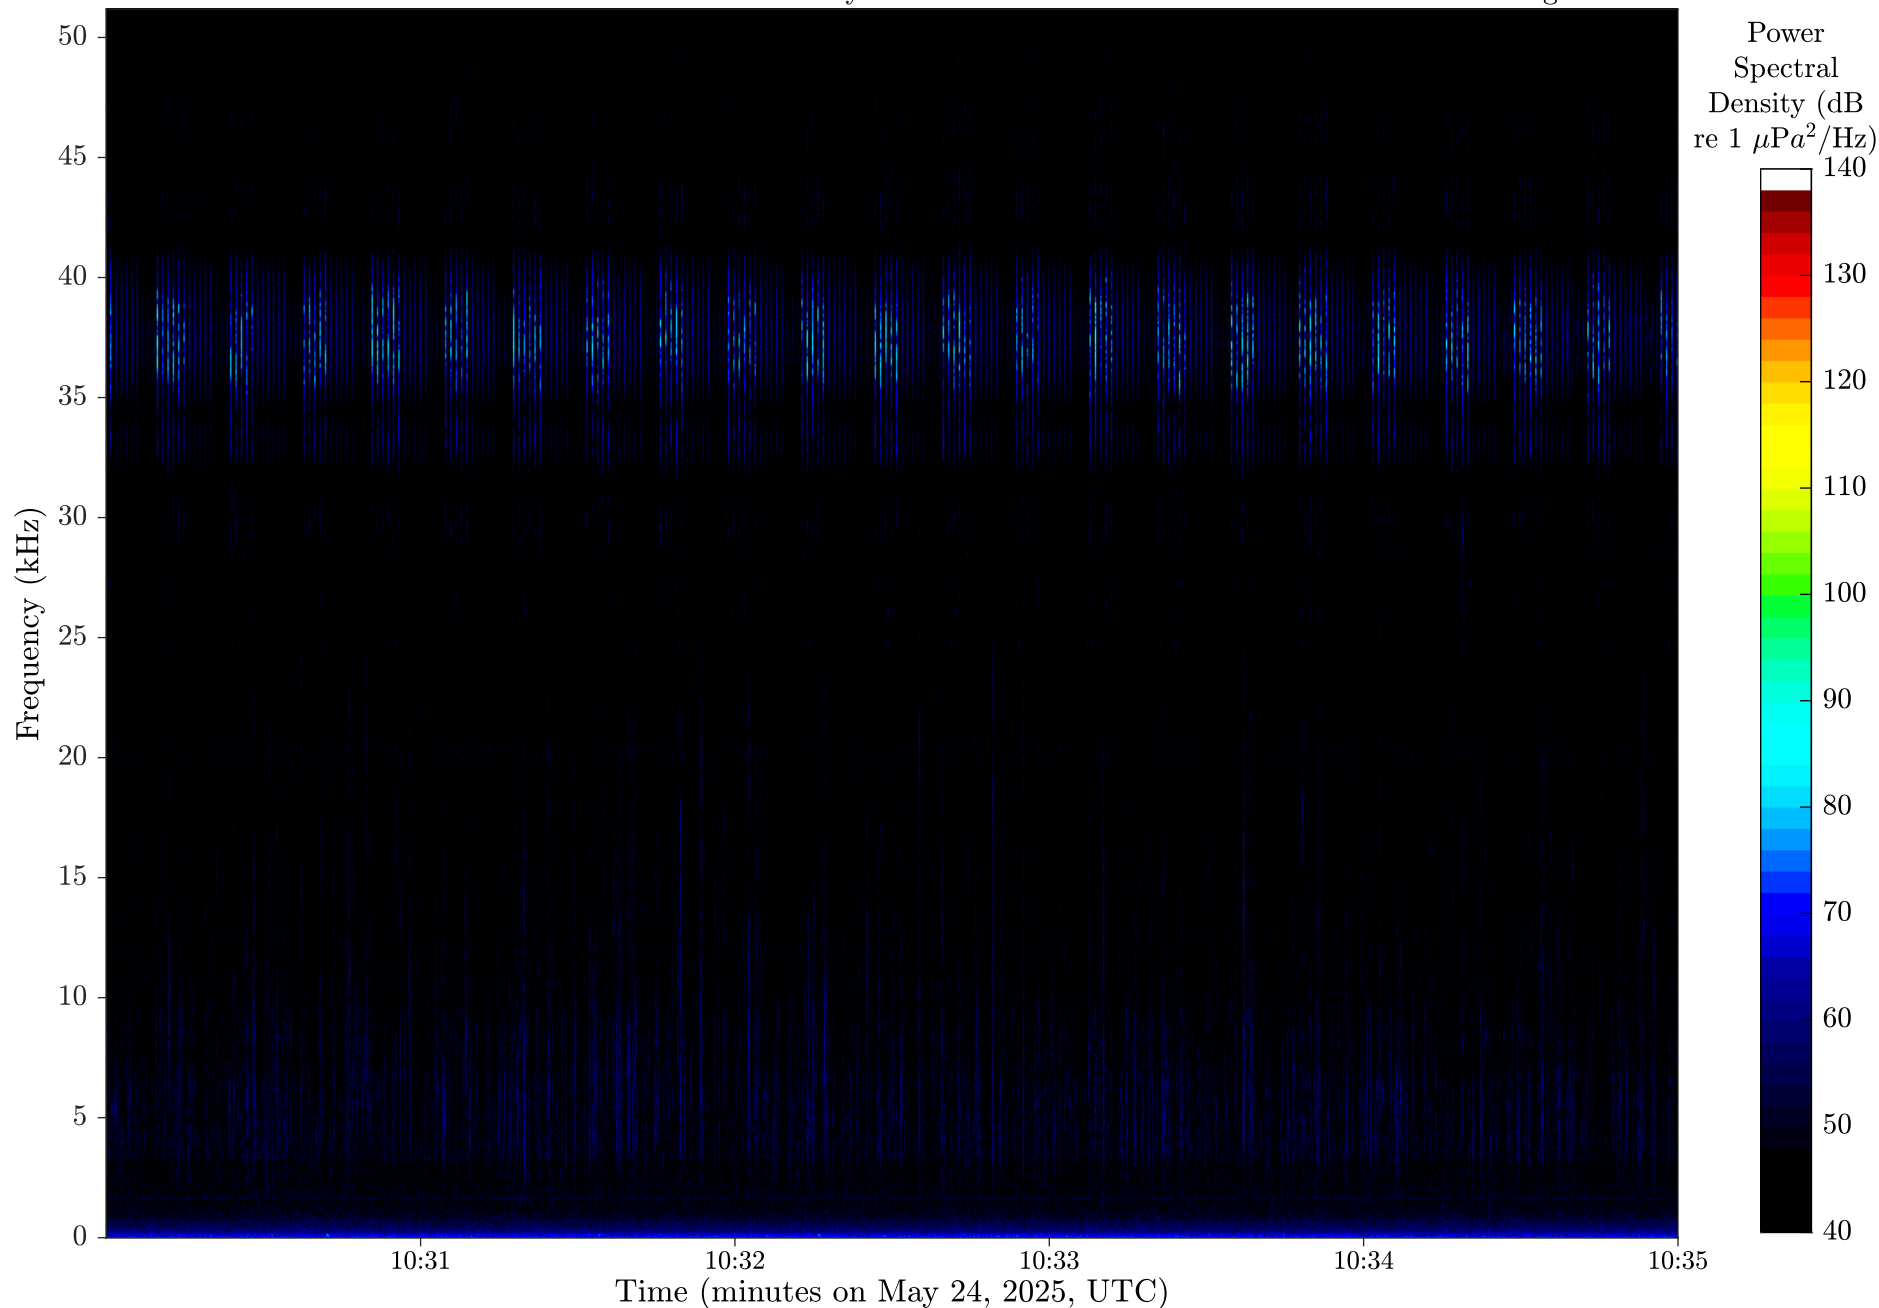

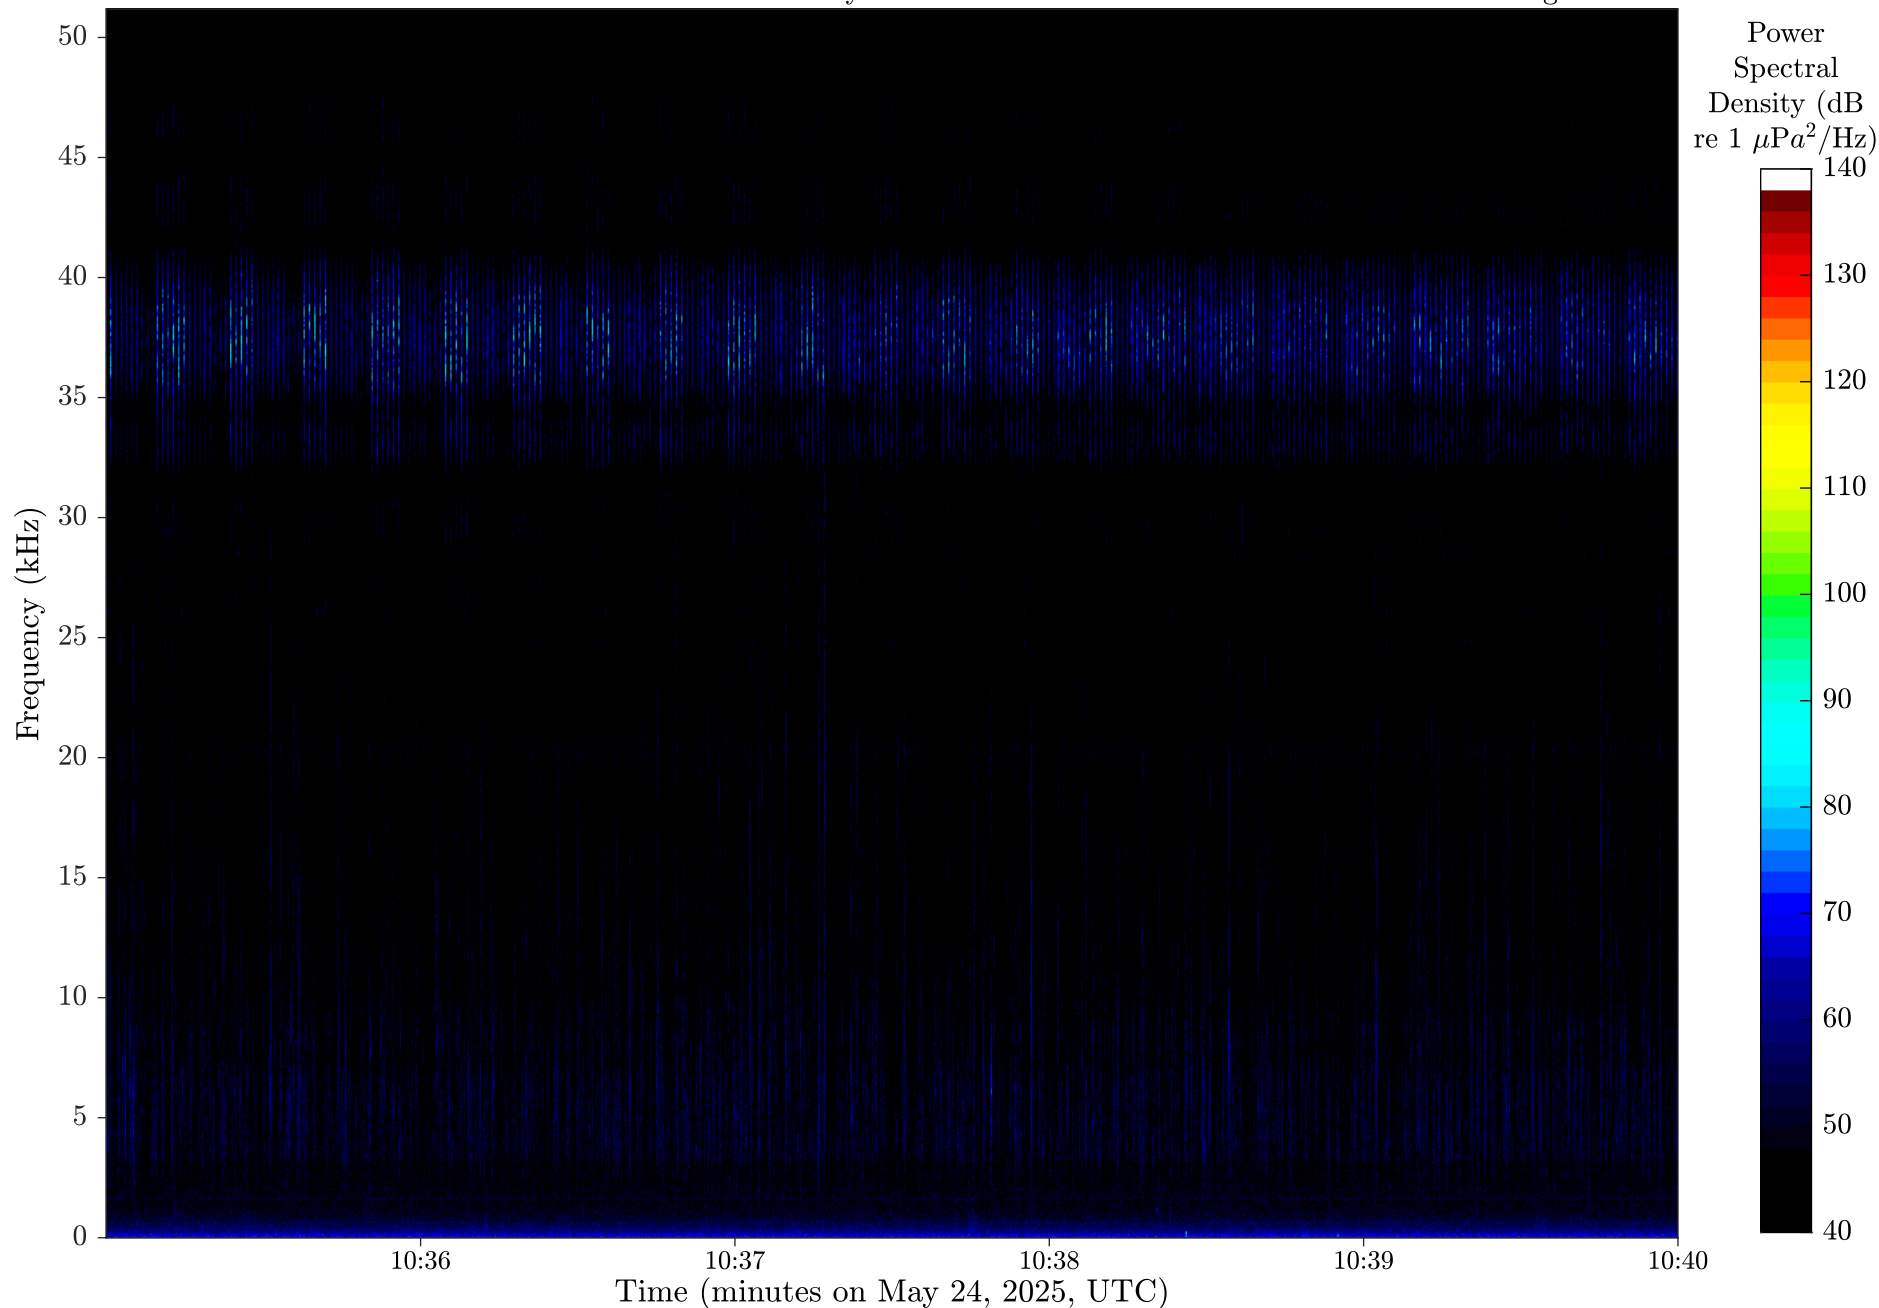


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:27:38 UTC

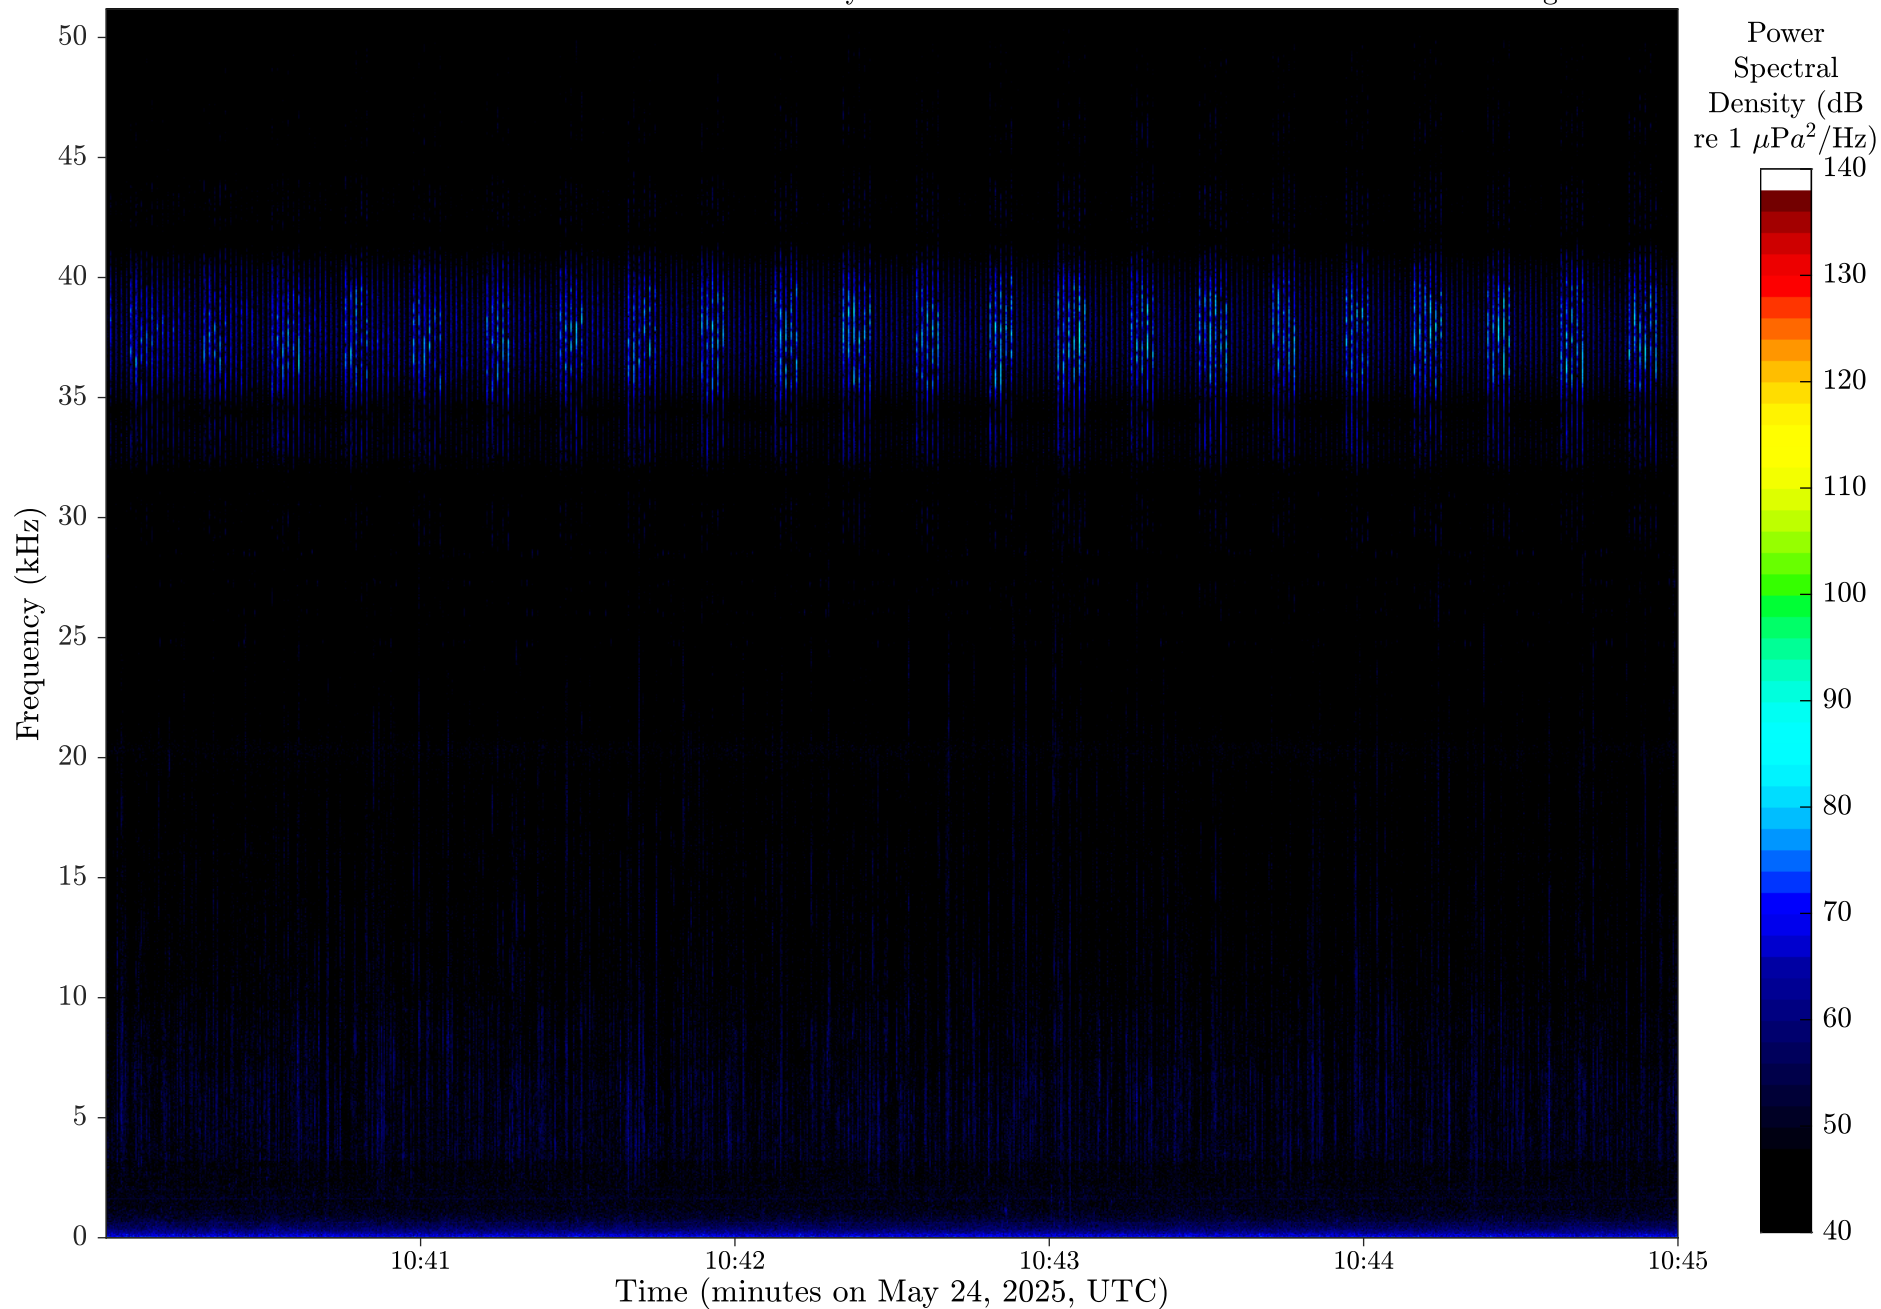

Comments: 33.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:27:46 UTC

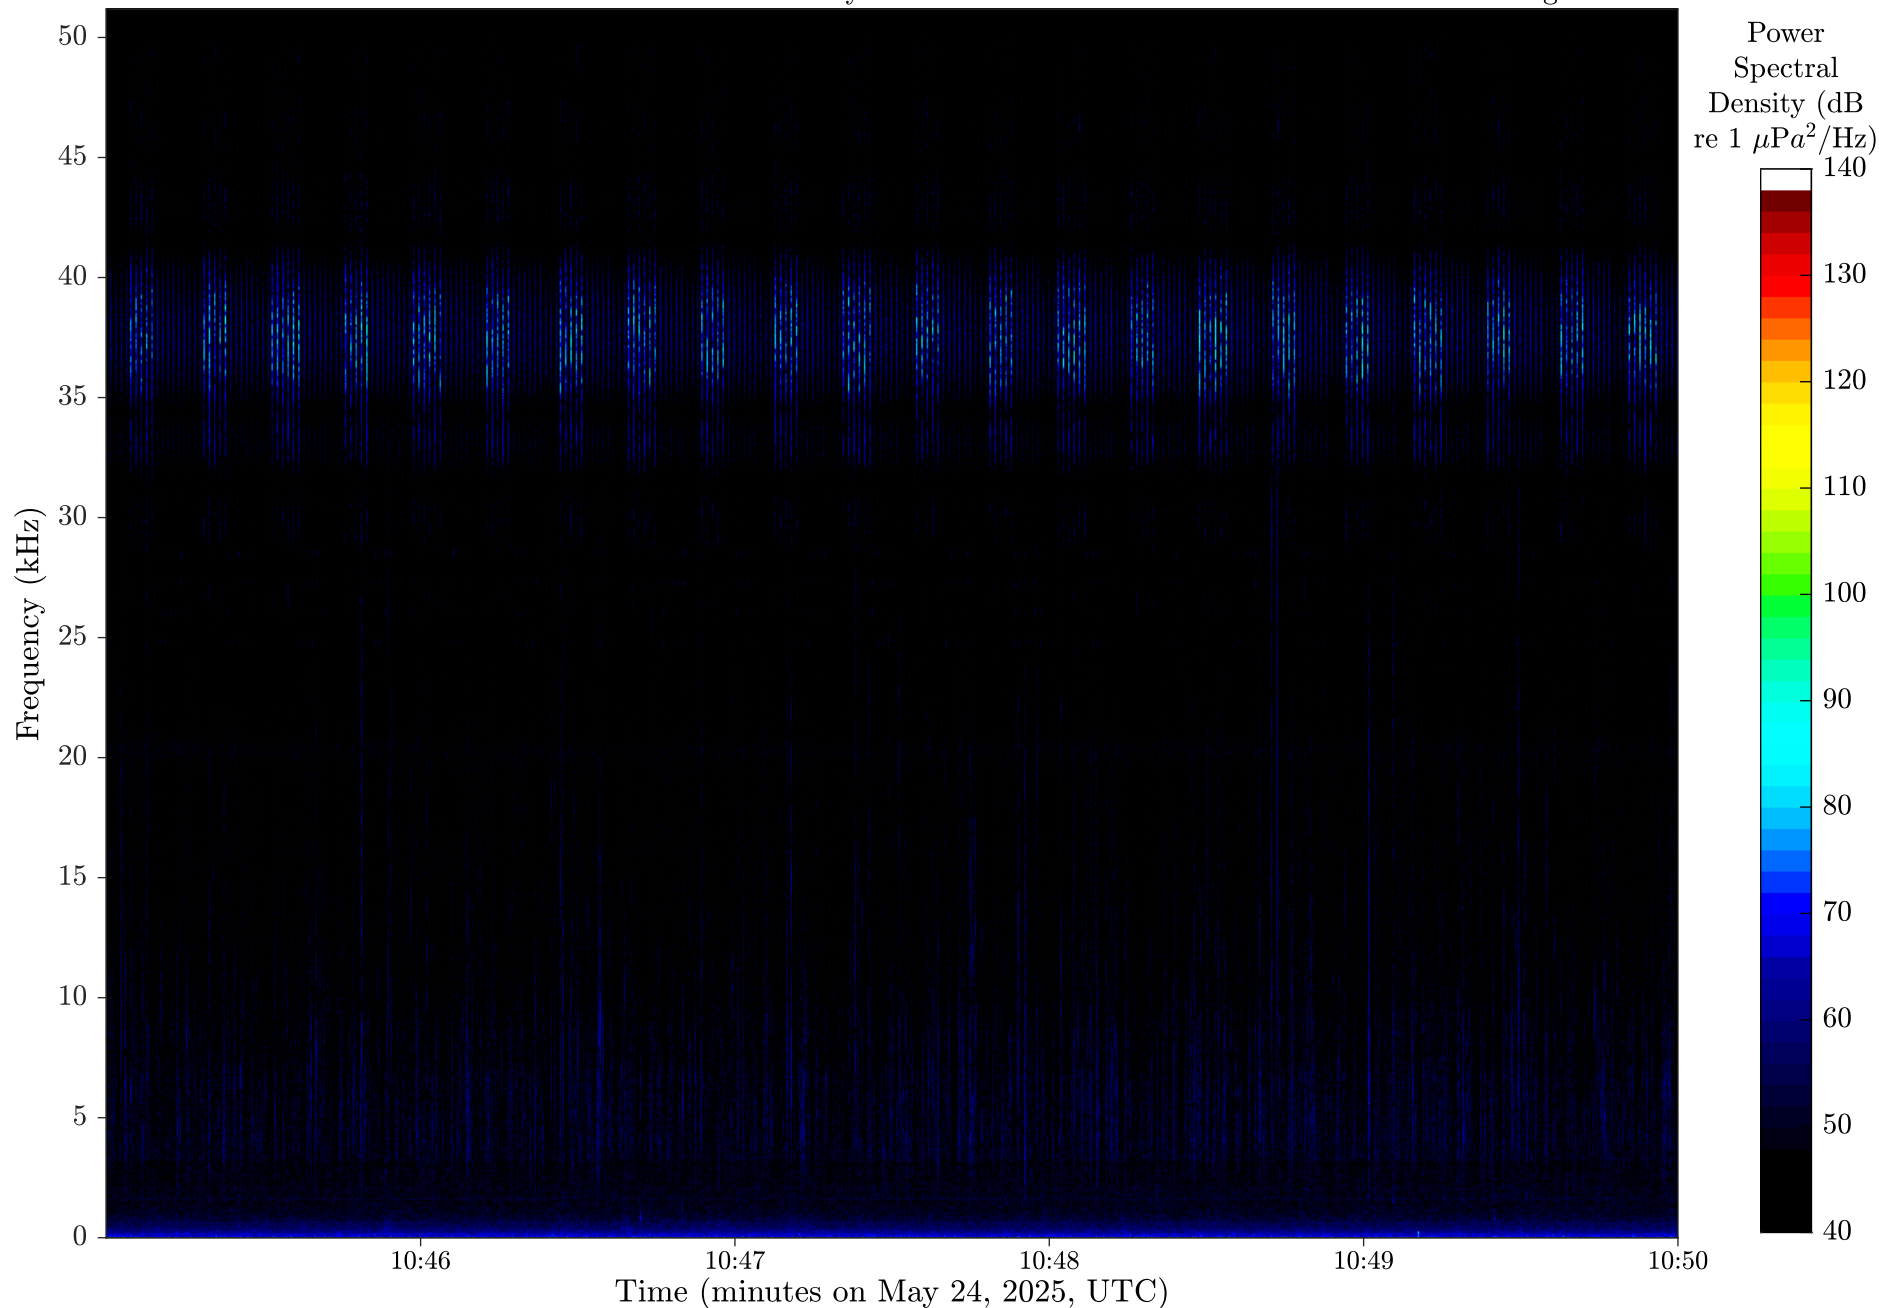


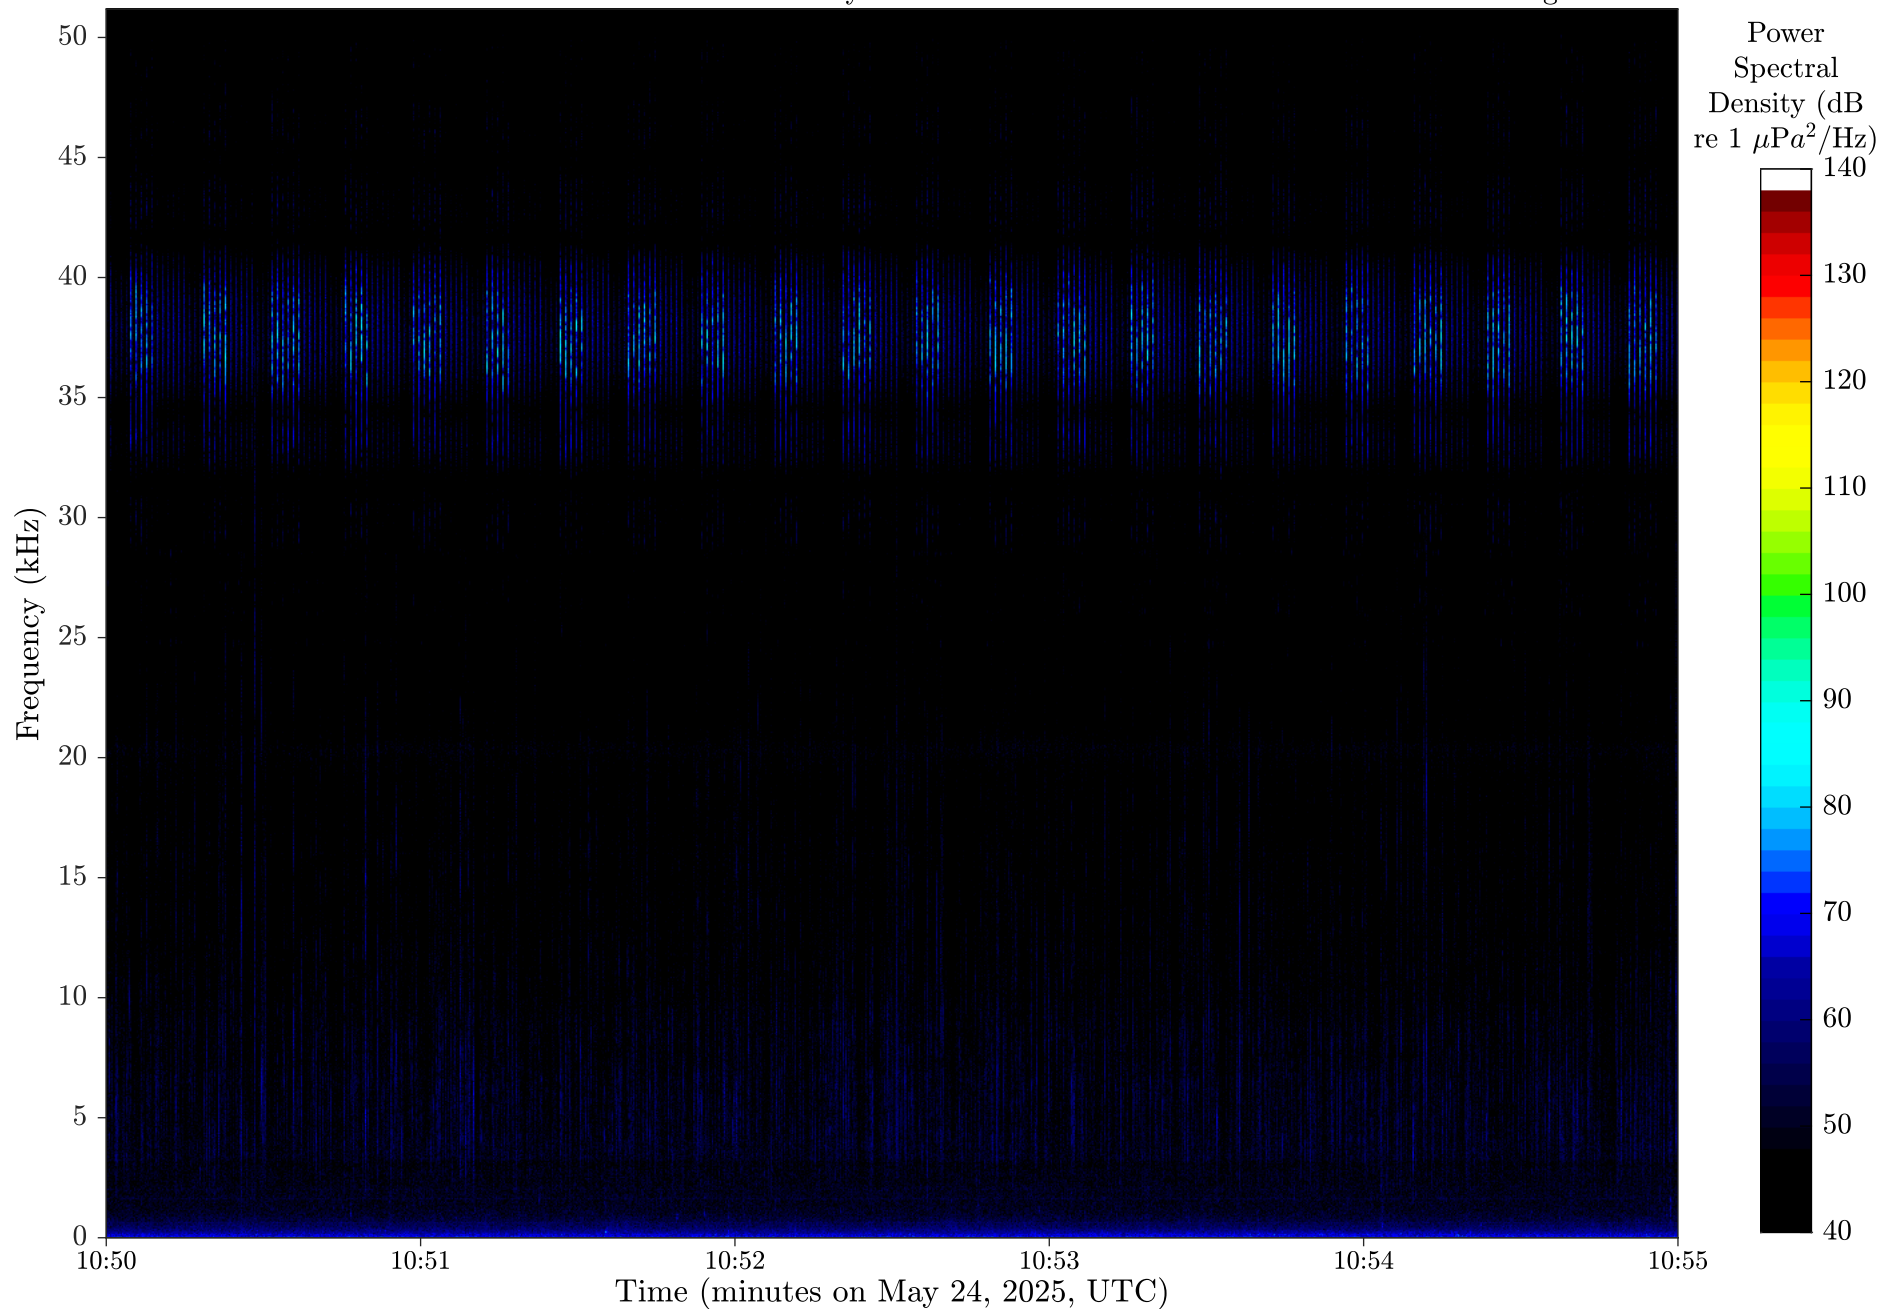

Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:28:00 UTC

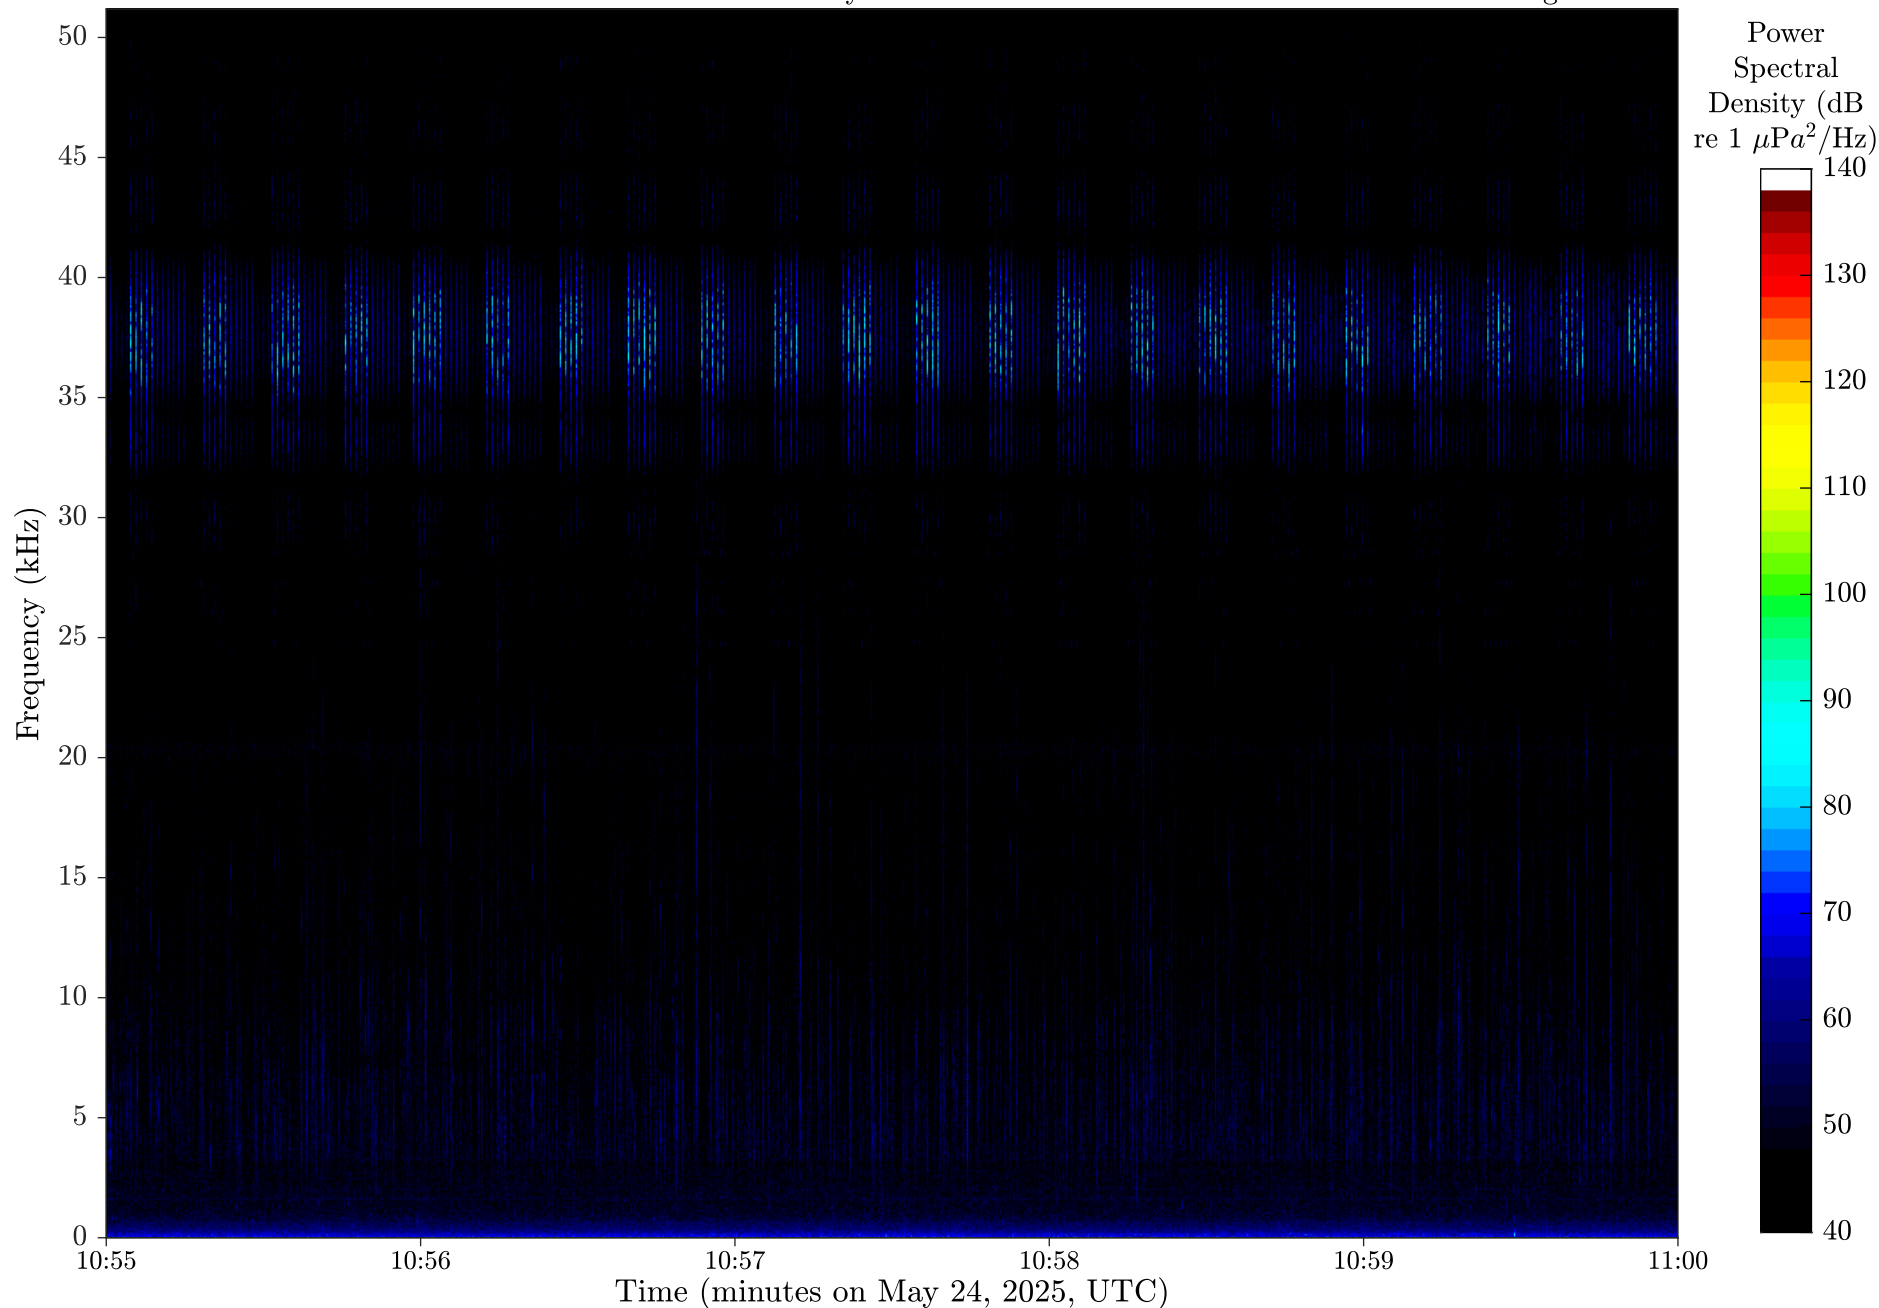

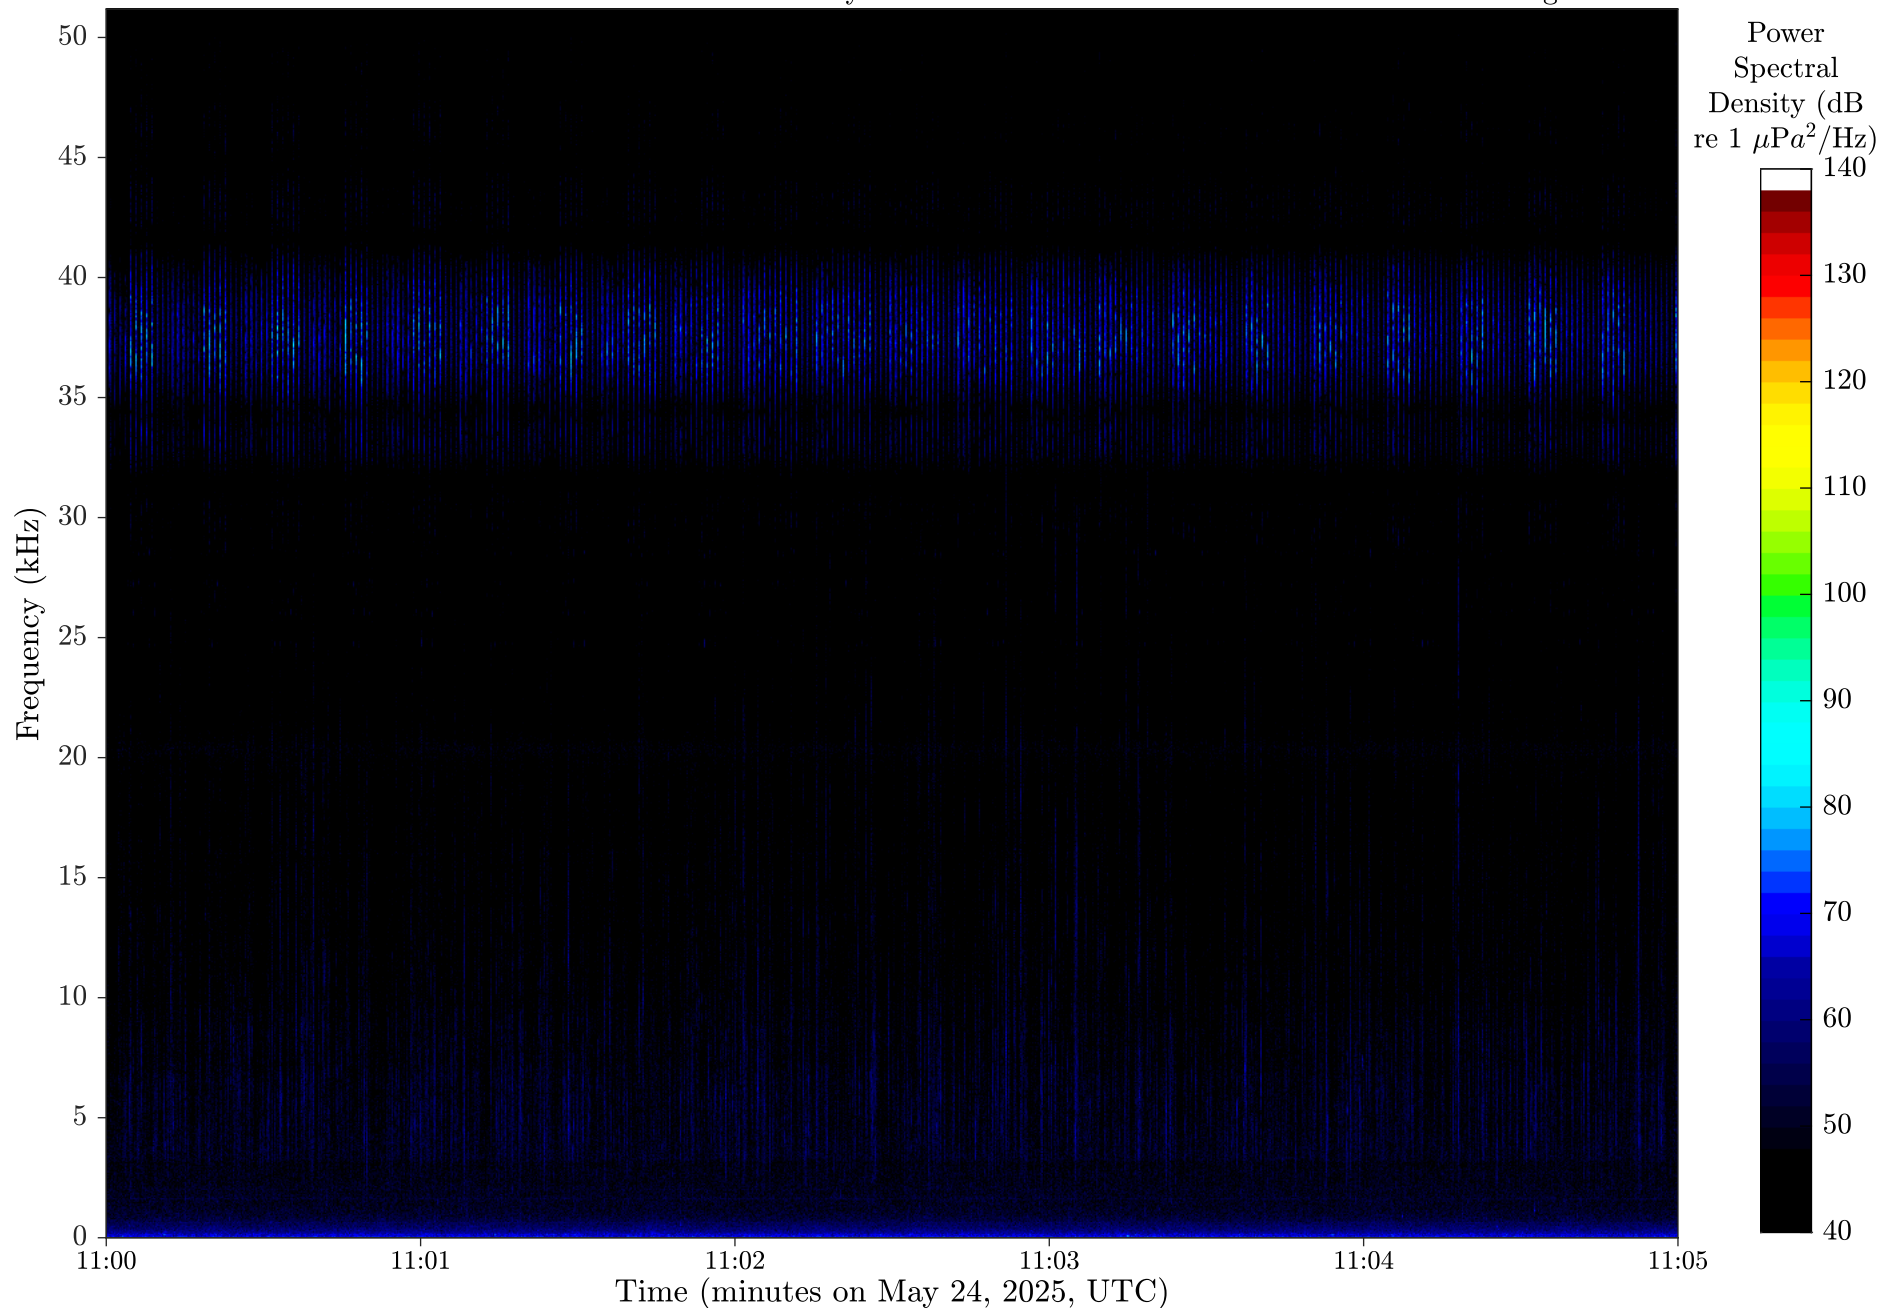


Comments: 32.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:28:15 UTC


Ocean Sonics icListen HF Hydrophone 1266 (23235)
Folger Passage • Folger Deep • 48.8139° N • 125.2746° W • 95 m
Start time: 24-May-2025 11:05:00.000 UTC • Data Diversion Mode: Original Data



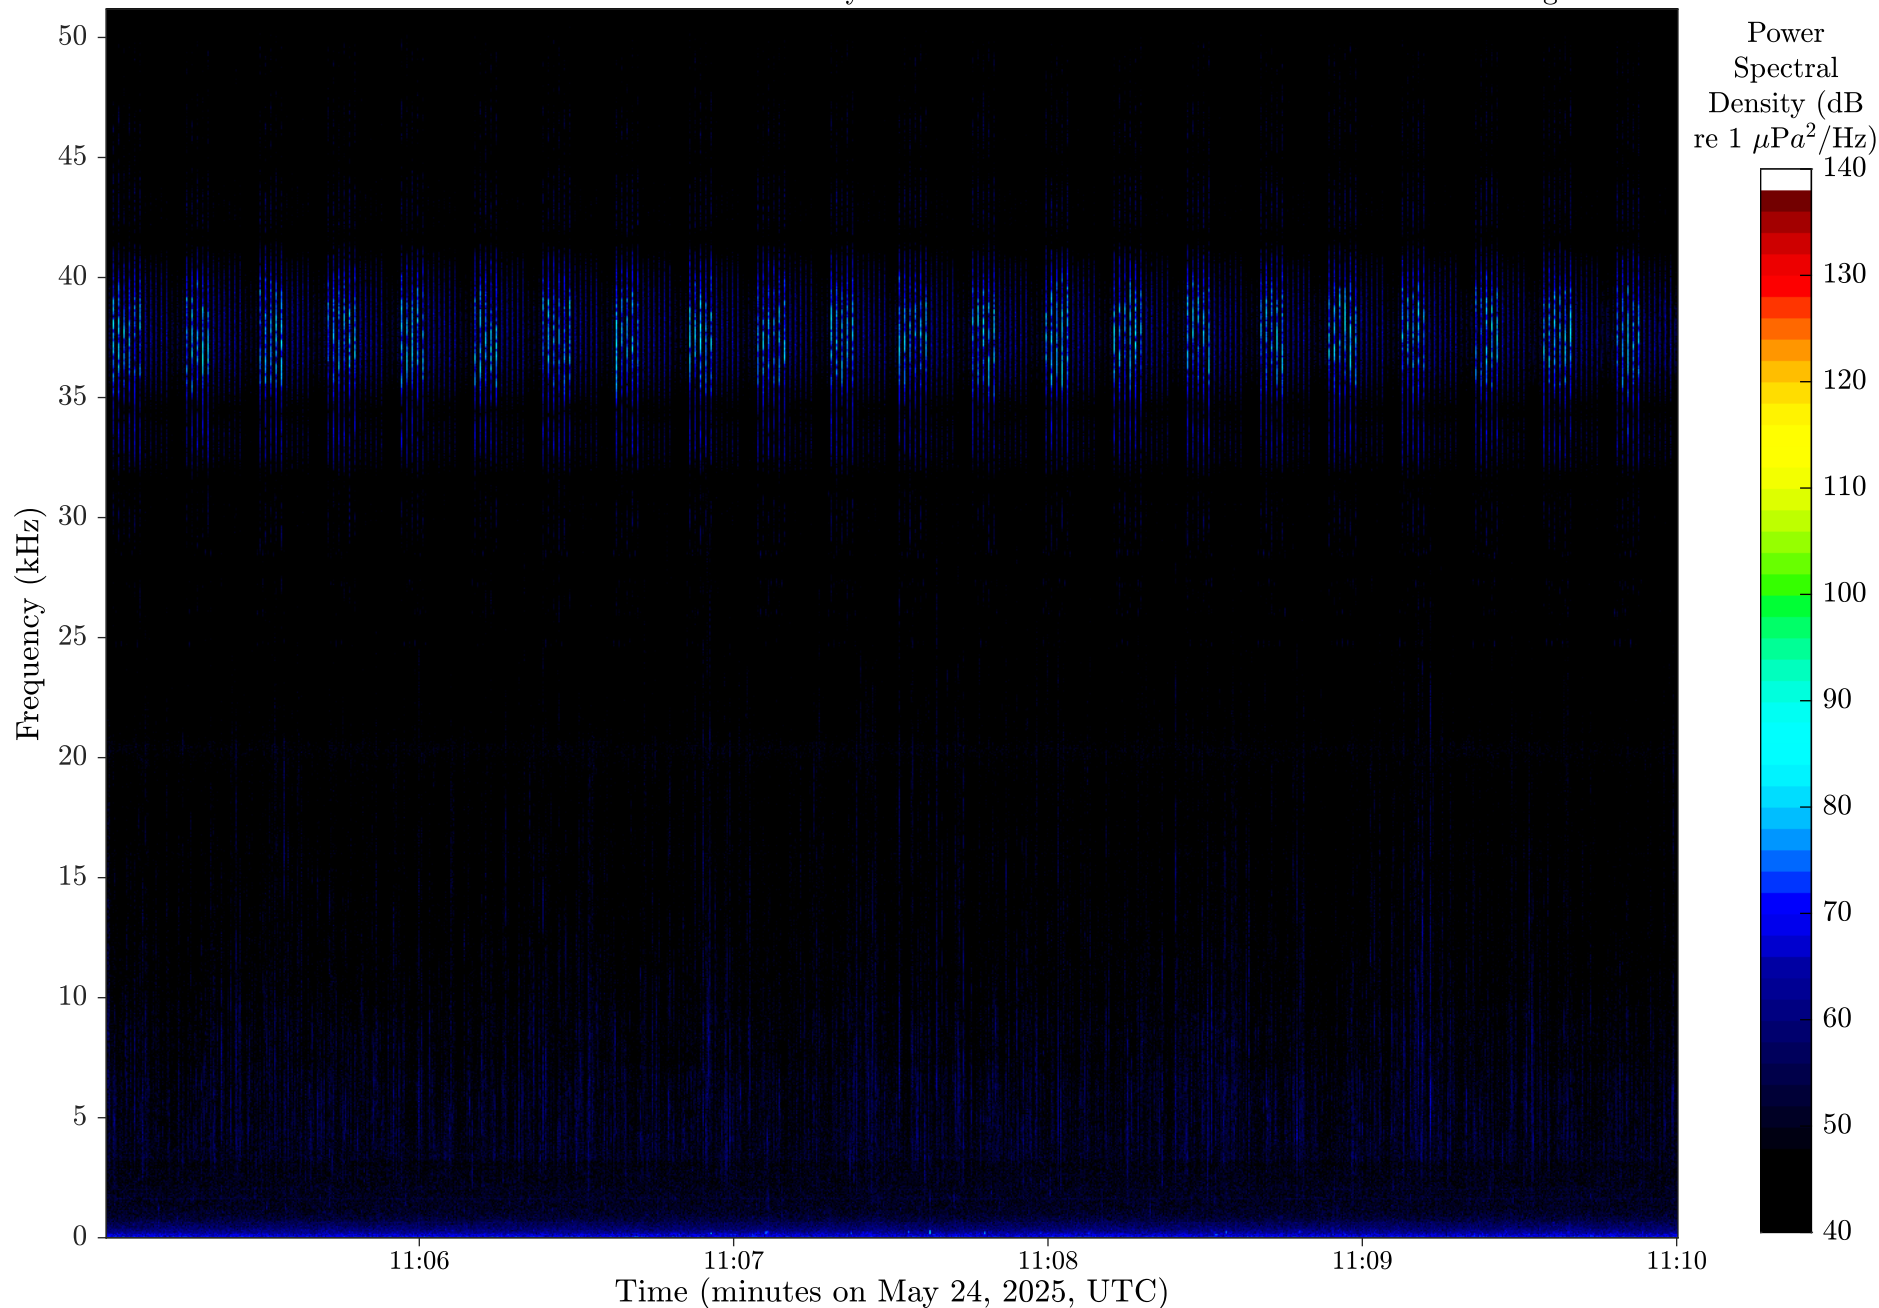


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:28:24 UTC

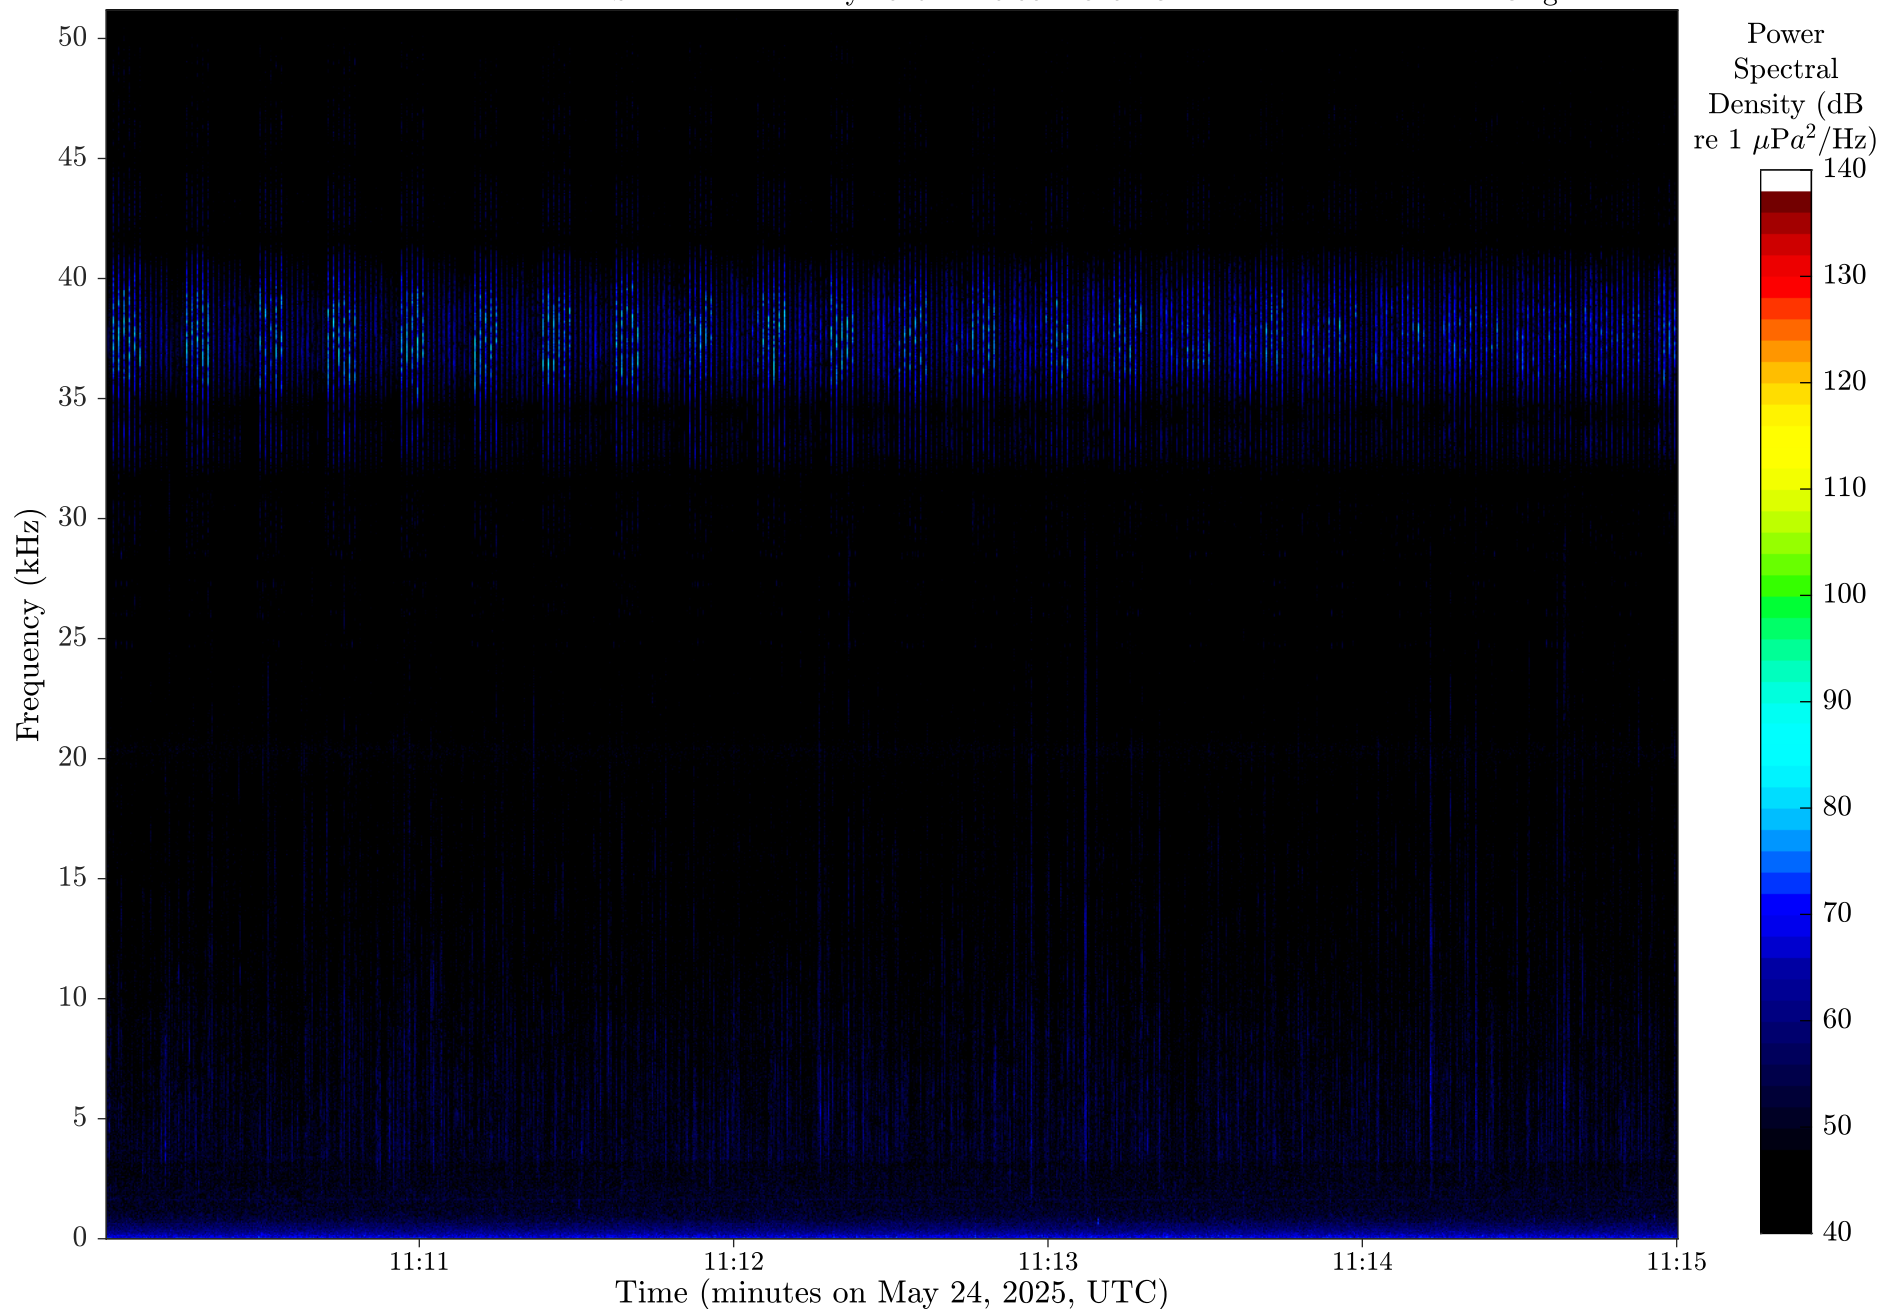


Comments: 32.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:28:31 UTC

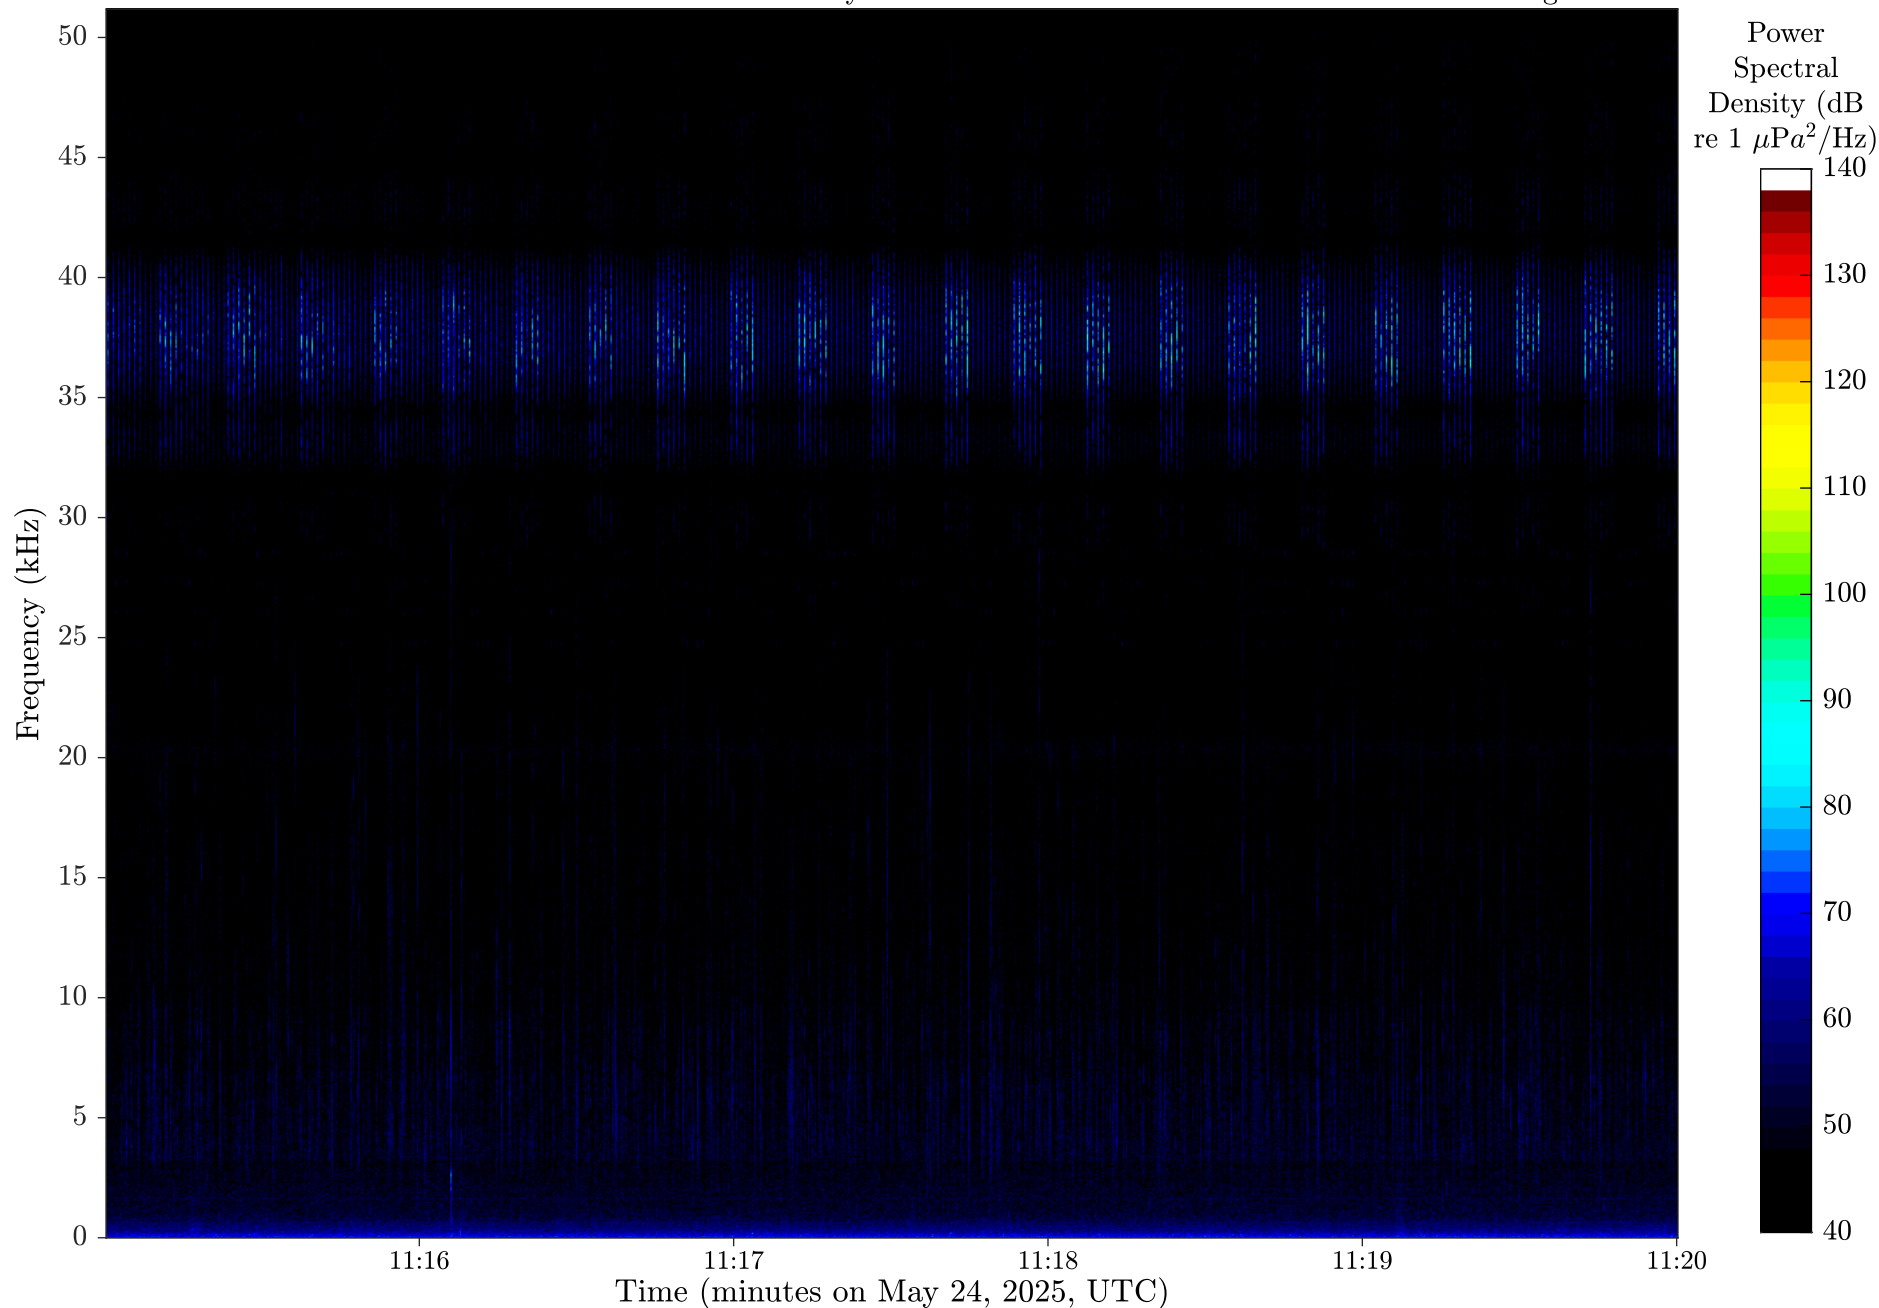

Comments: 31.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:28:39 UTC

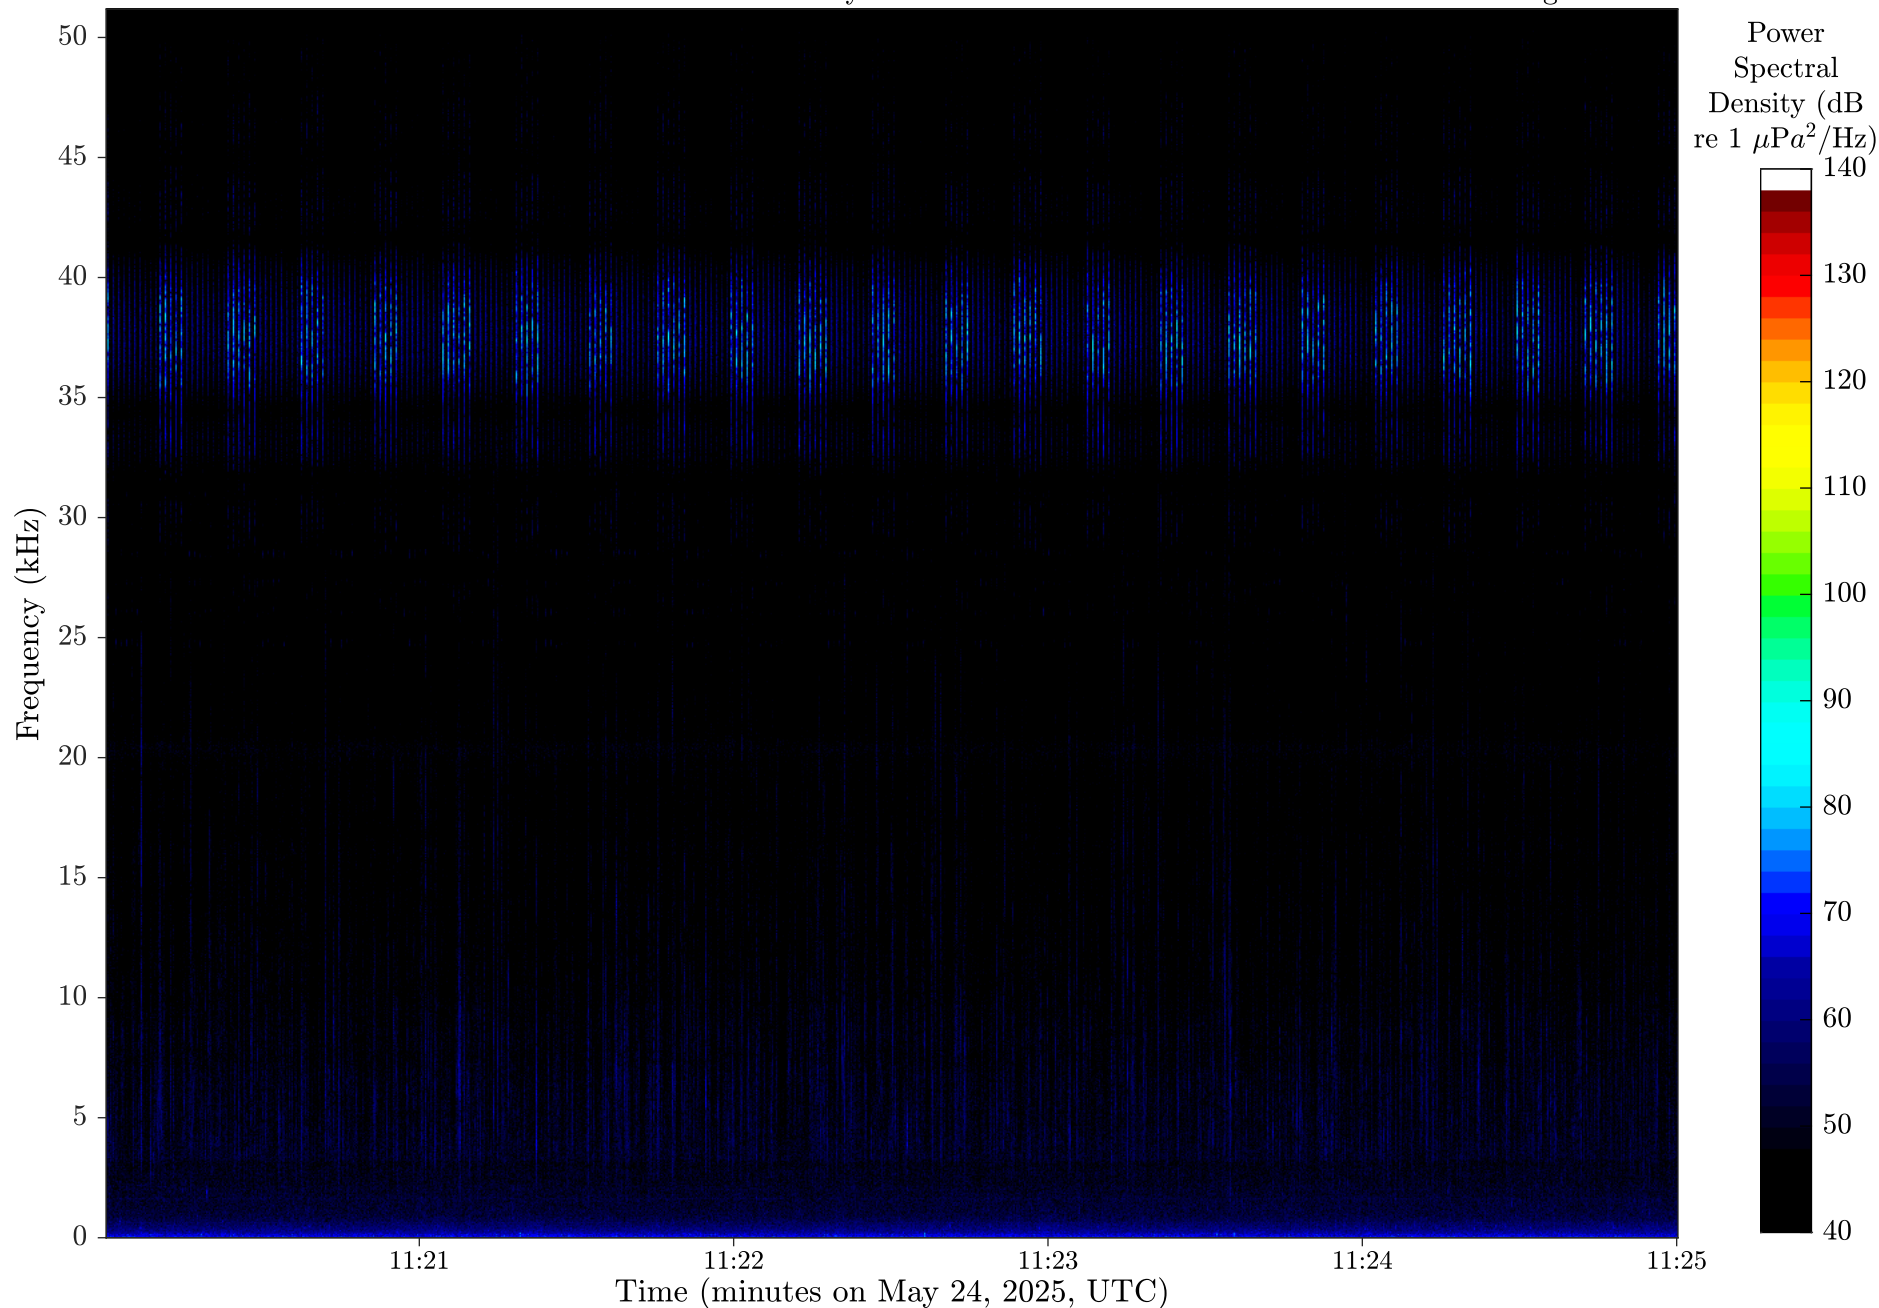

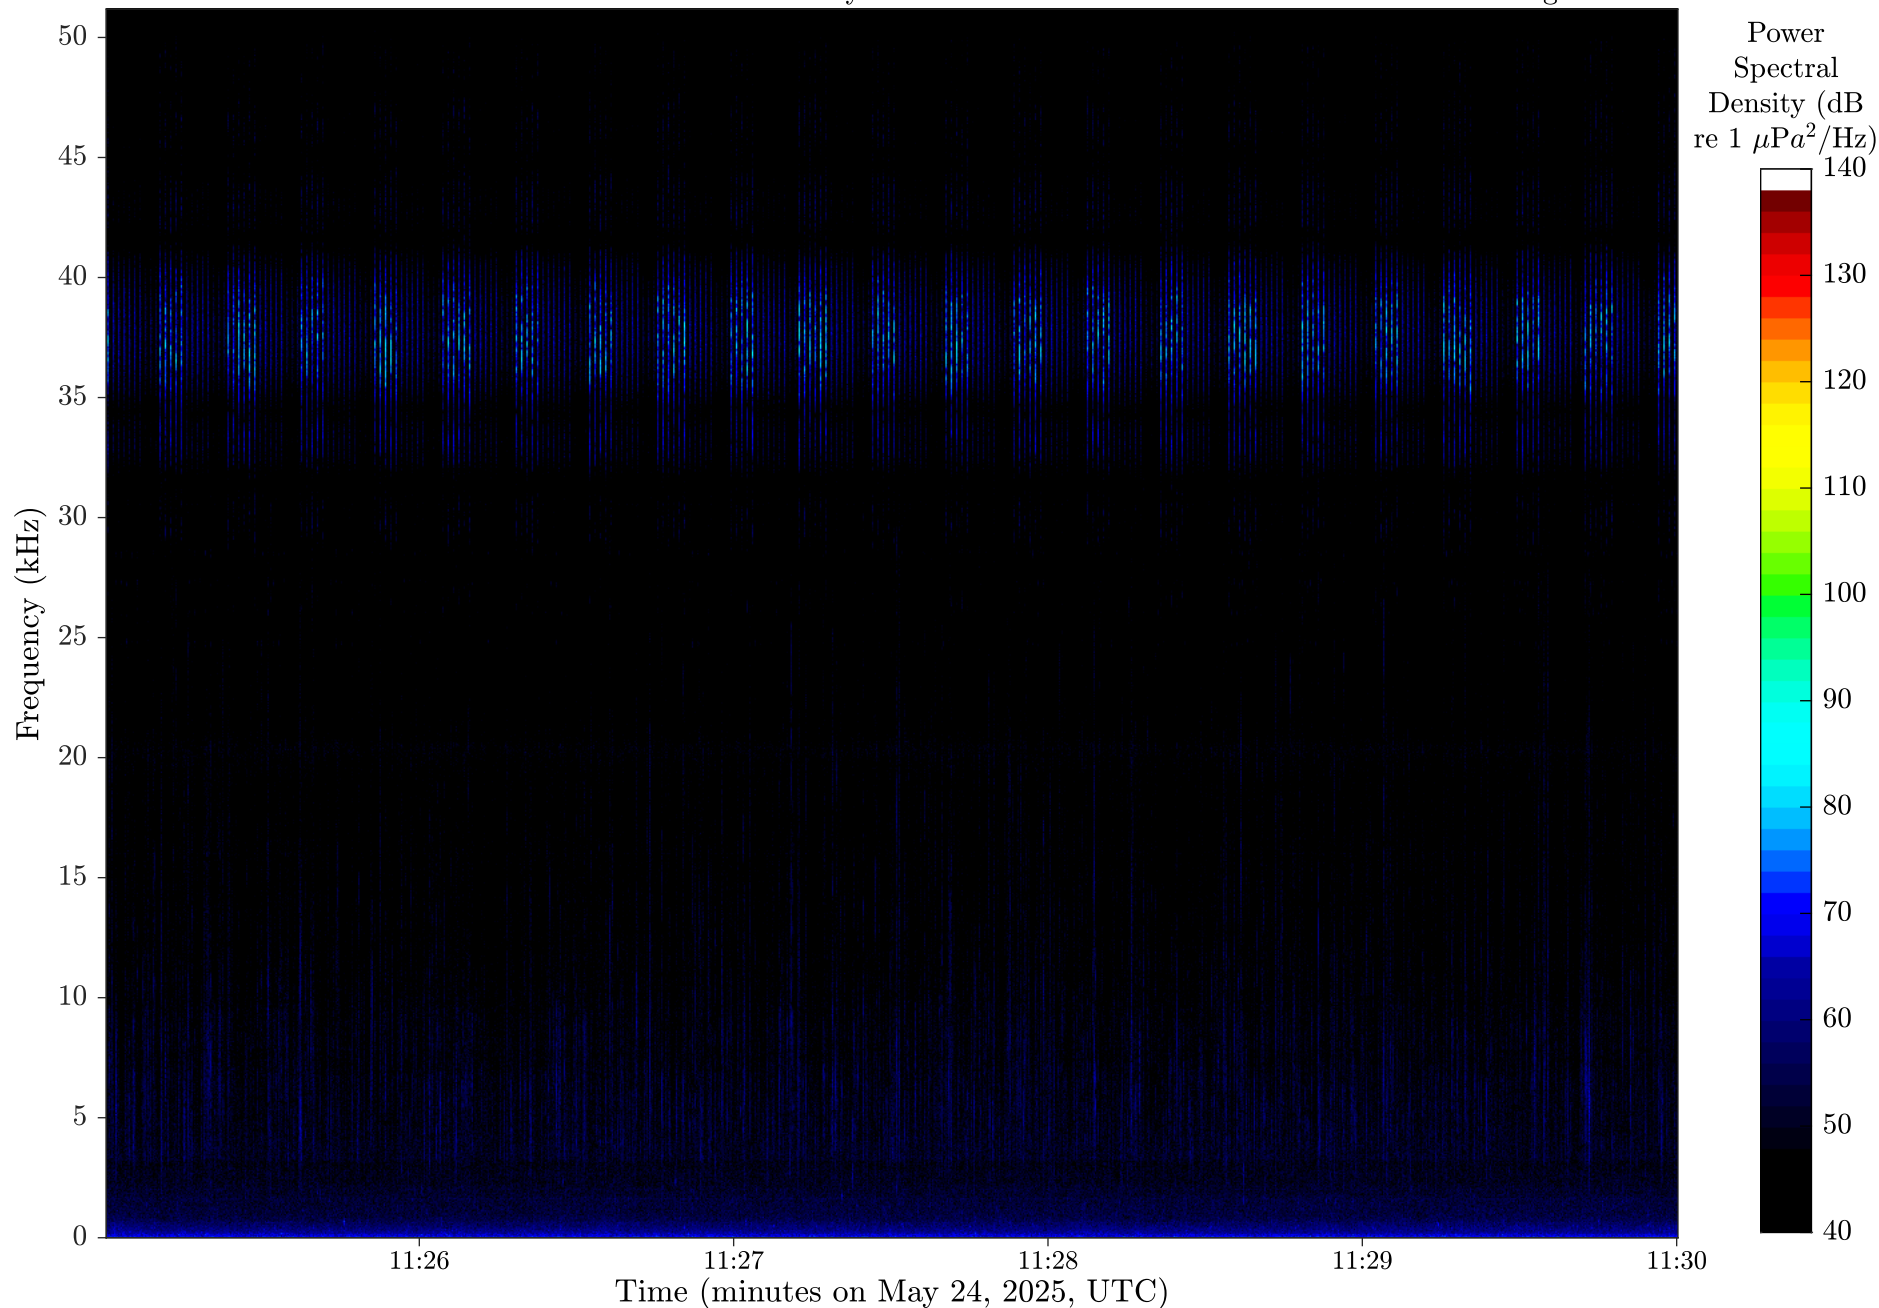


Comments: 32.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:28:54 UTC

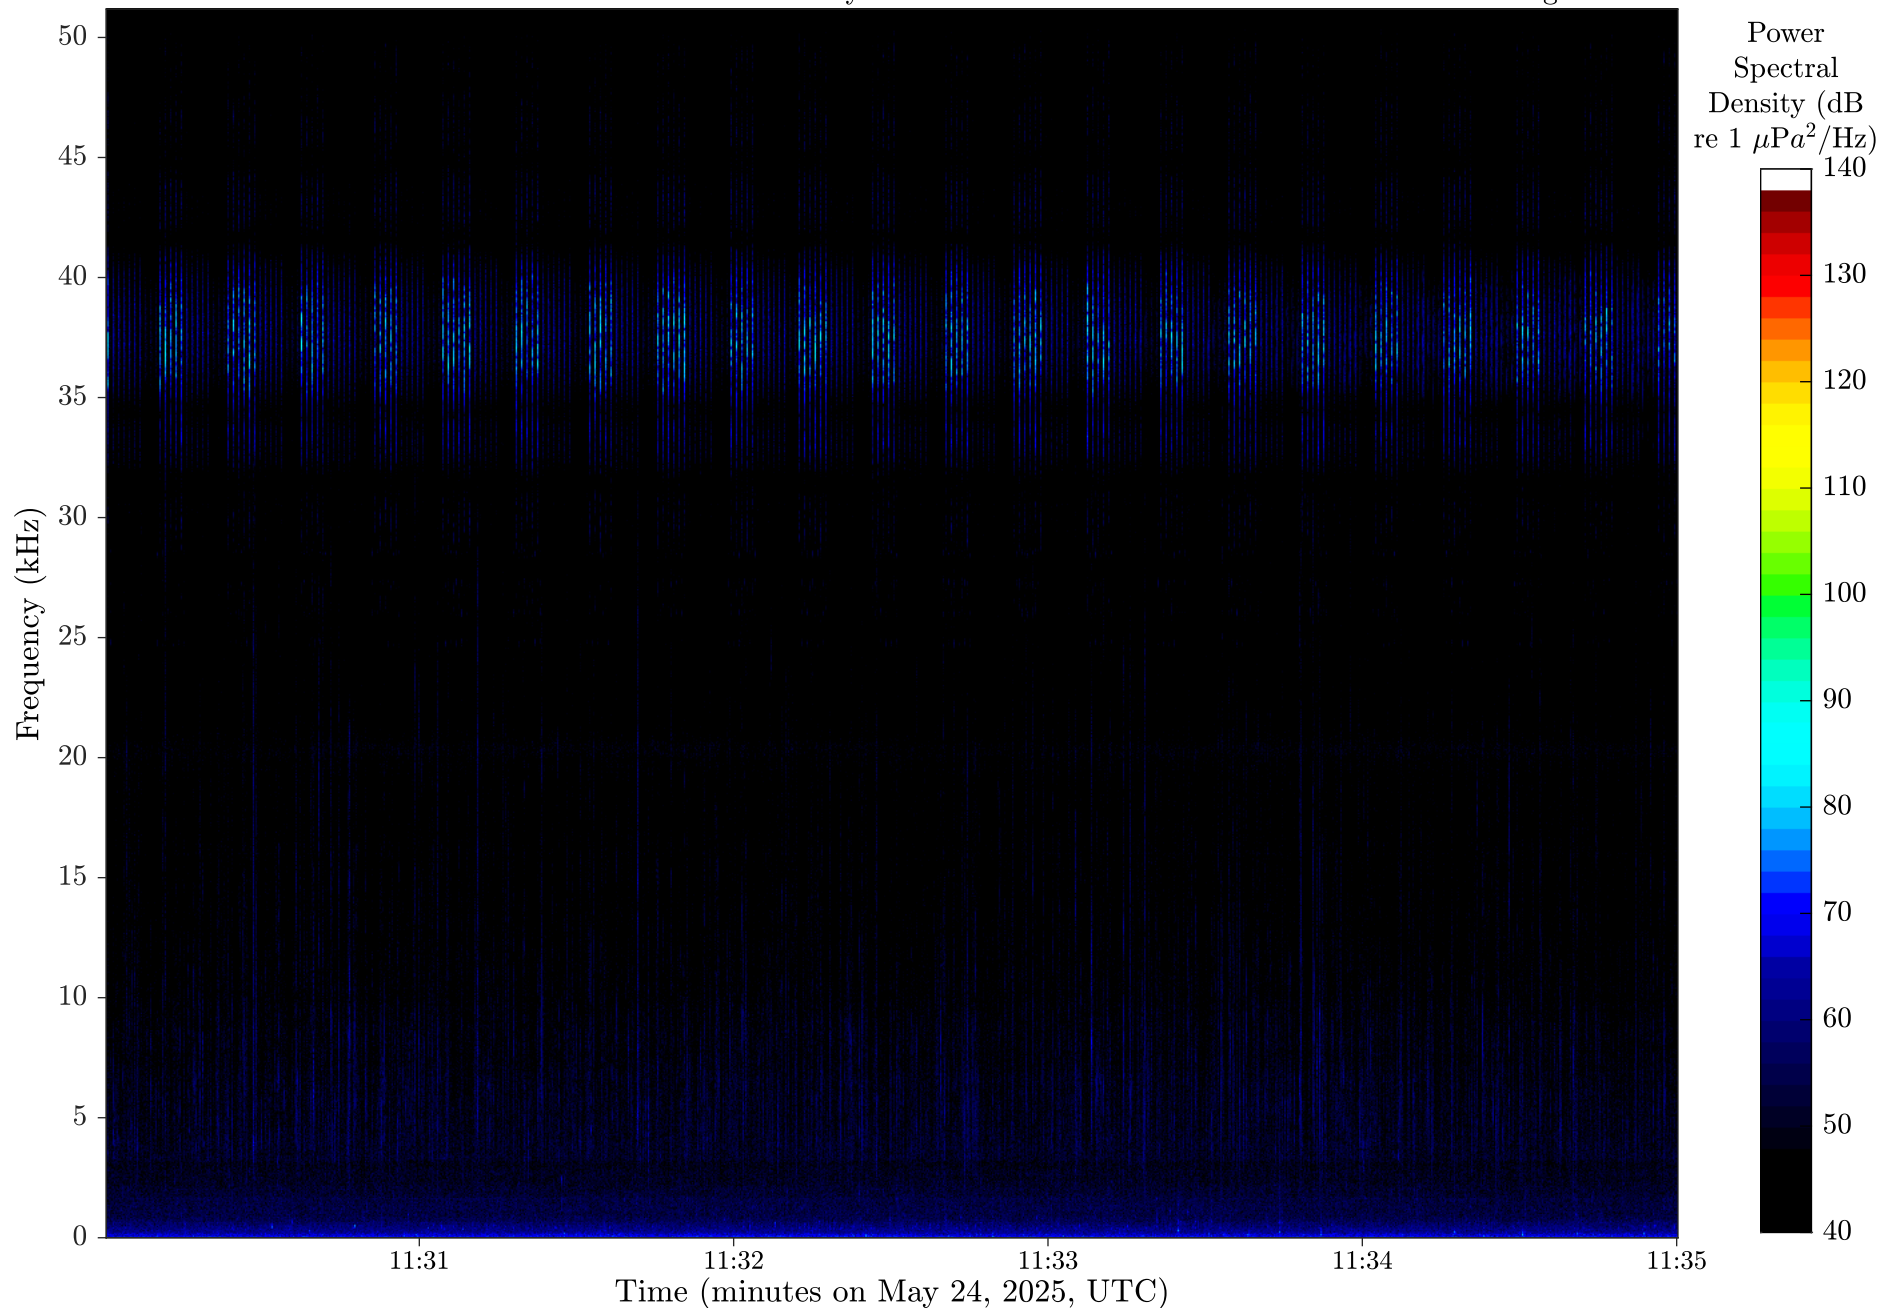


Comments: 32.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:01 UTC

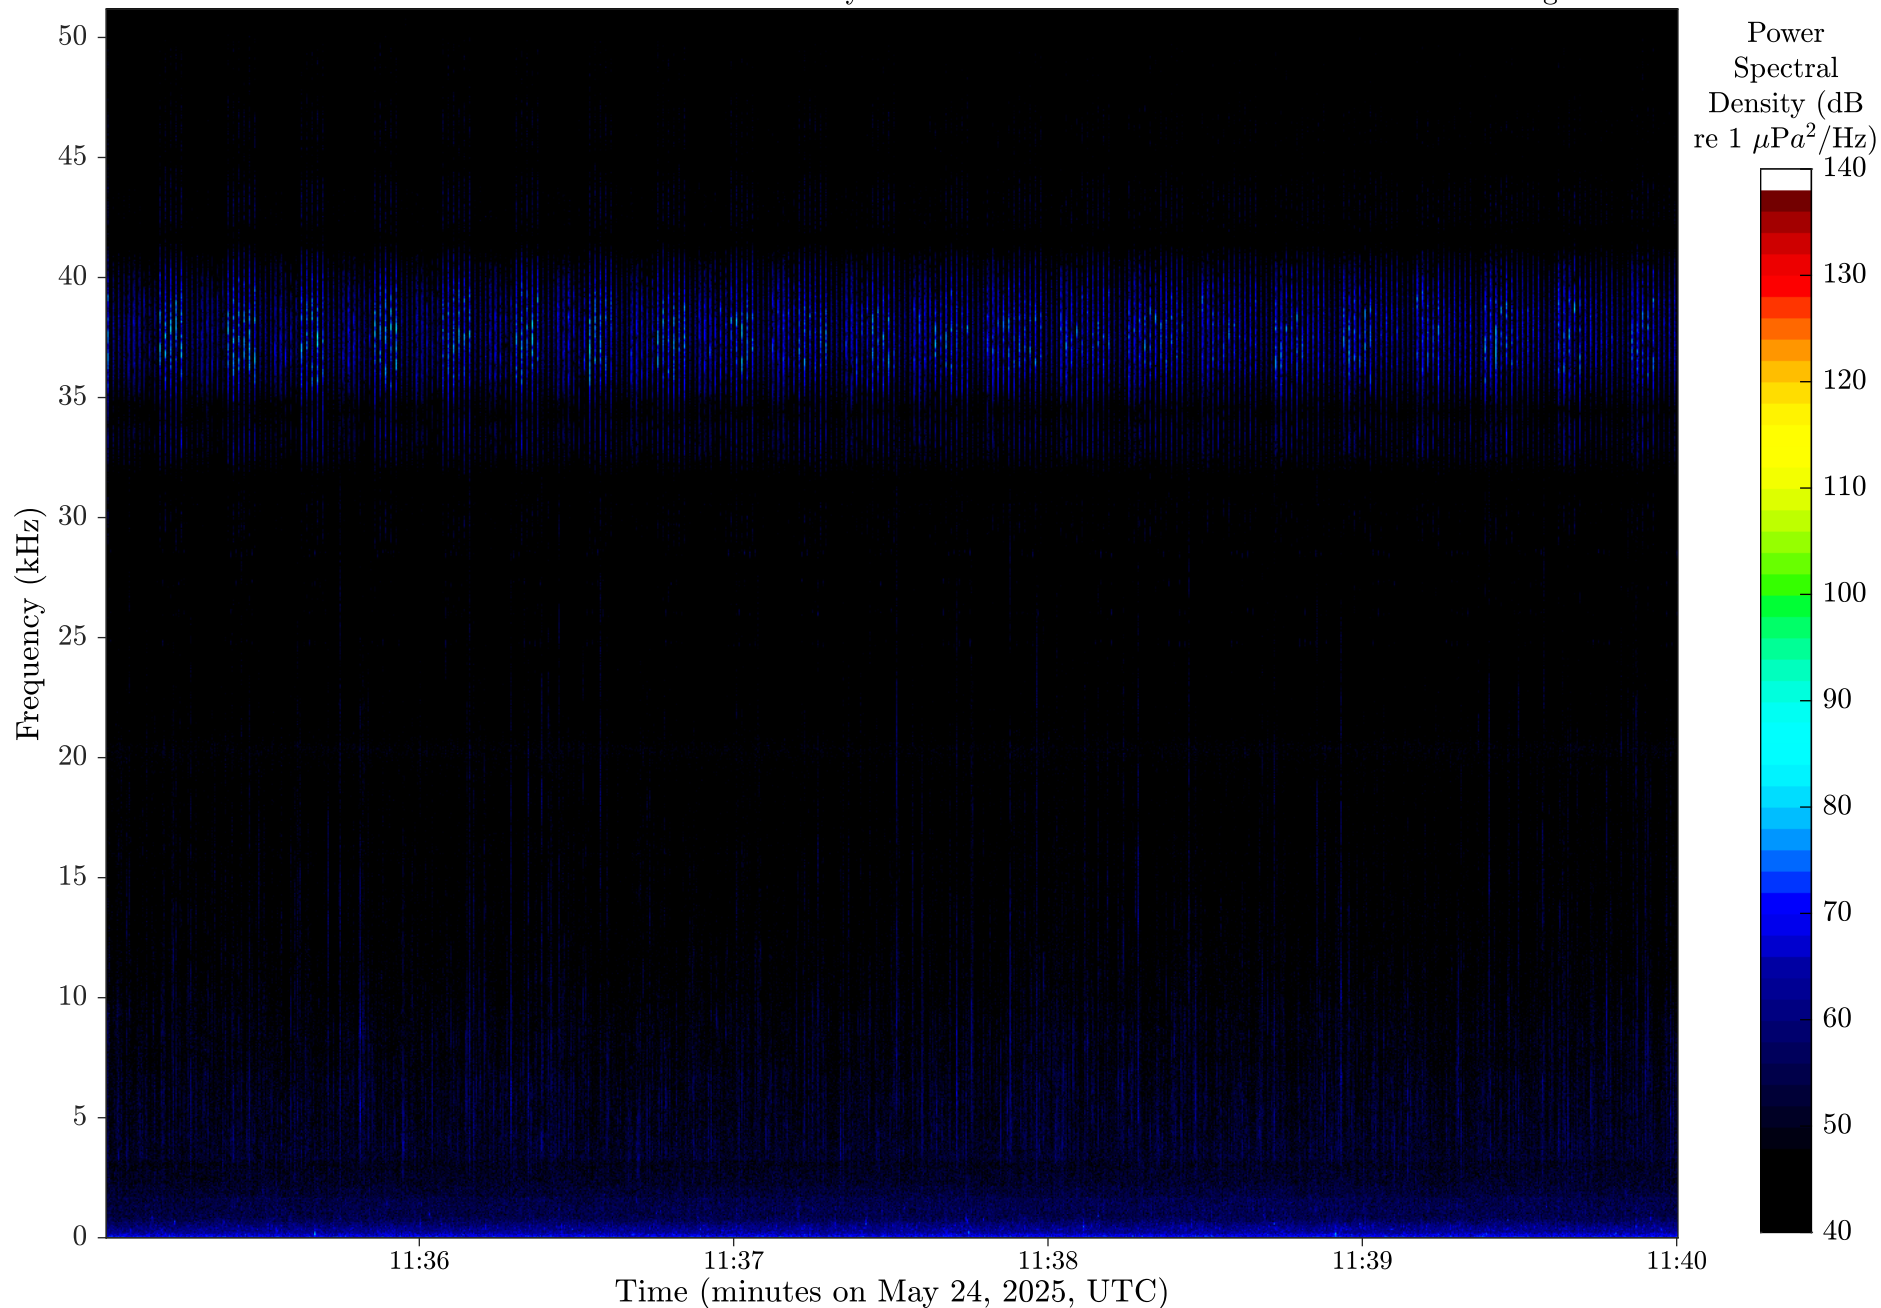


Comments: 30.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:29:09 UTC

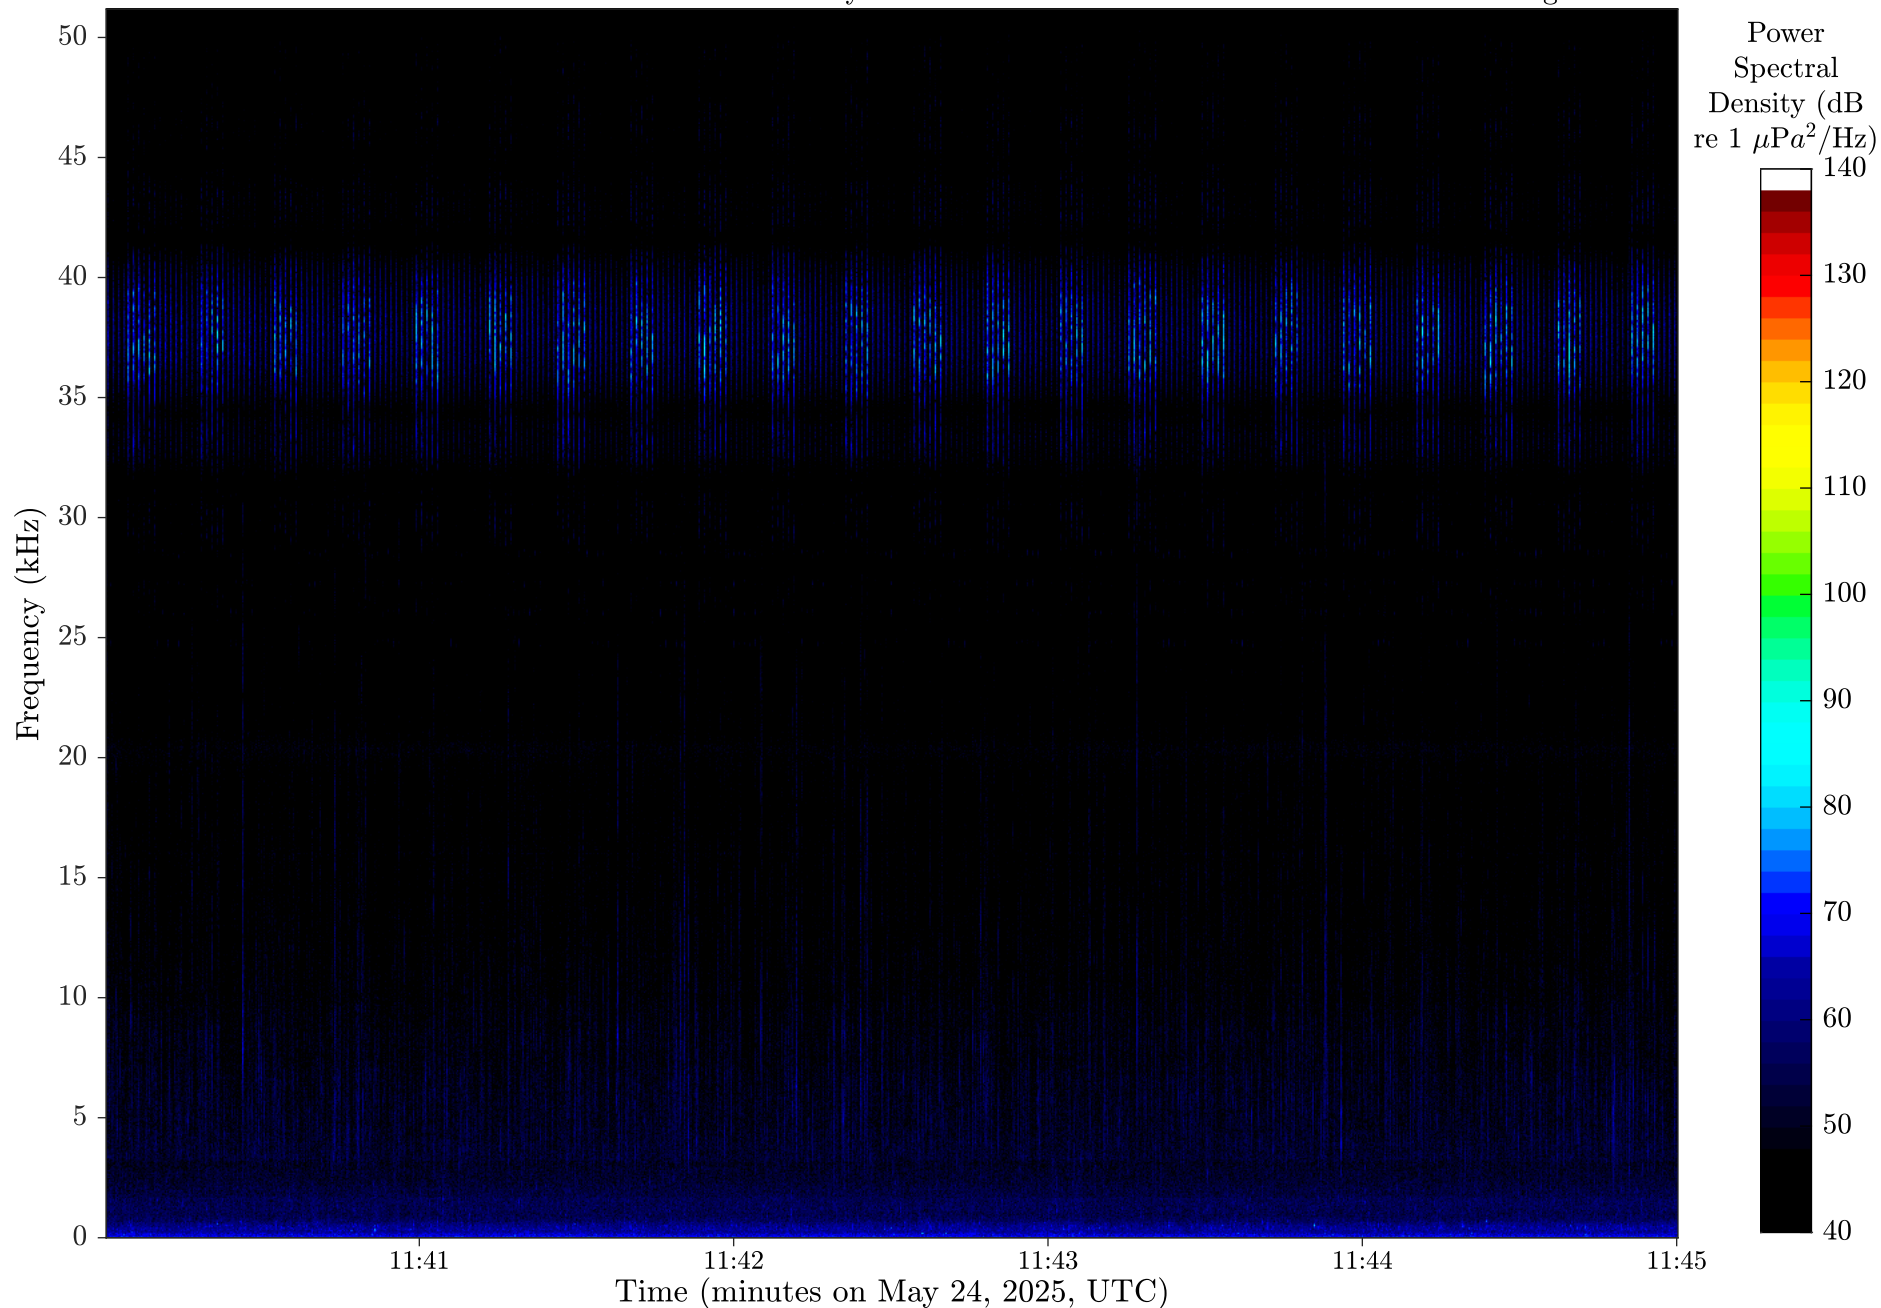

Comments: 30.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:29:15 UTC

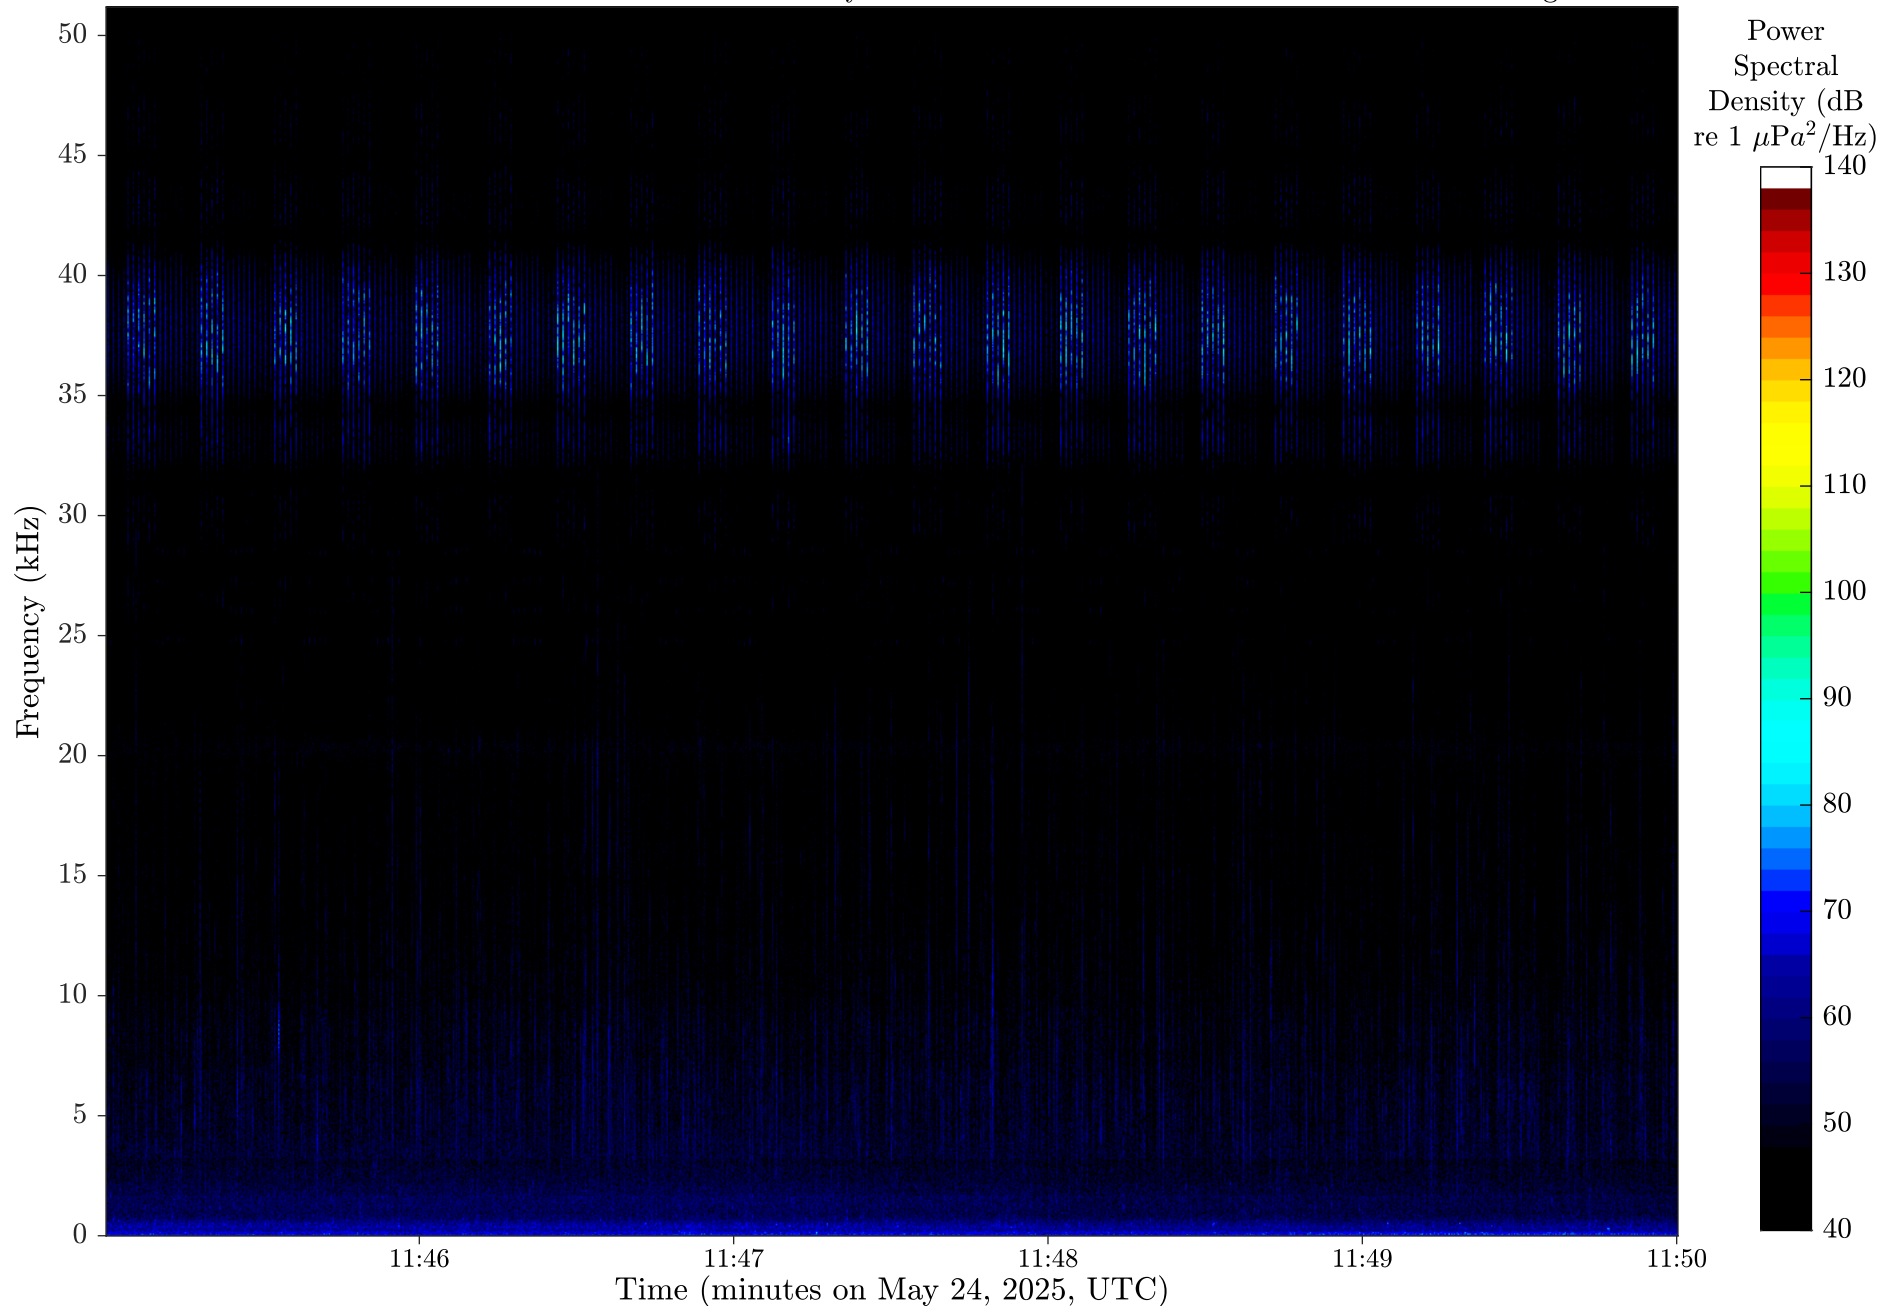

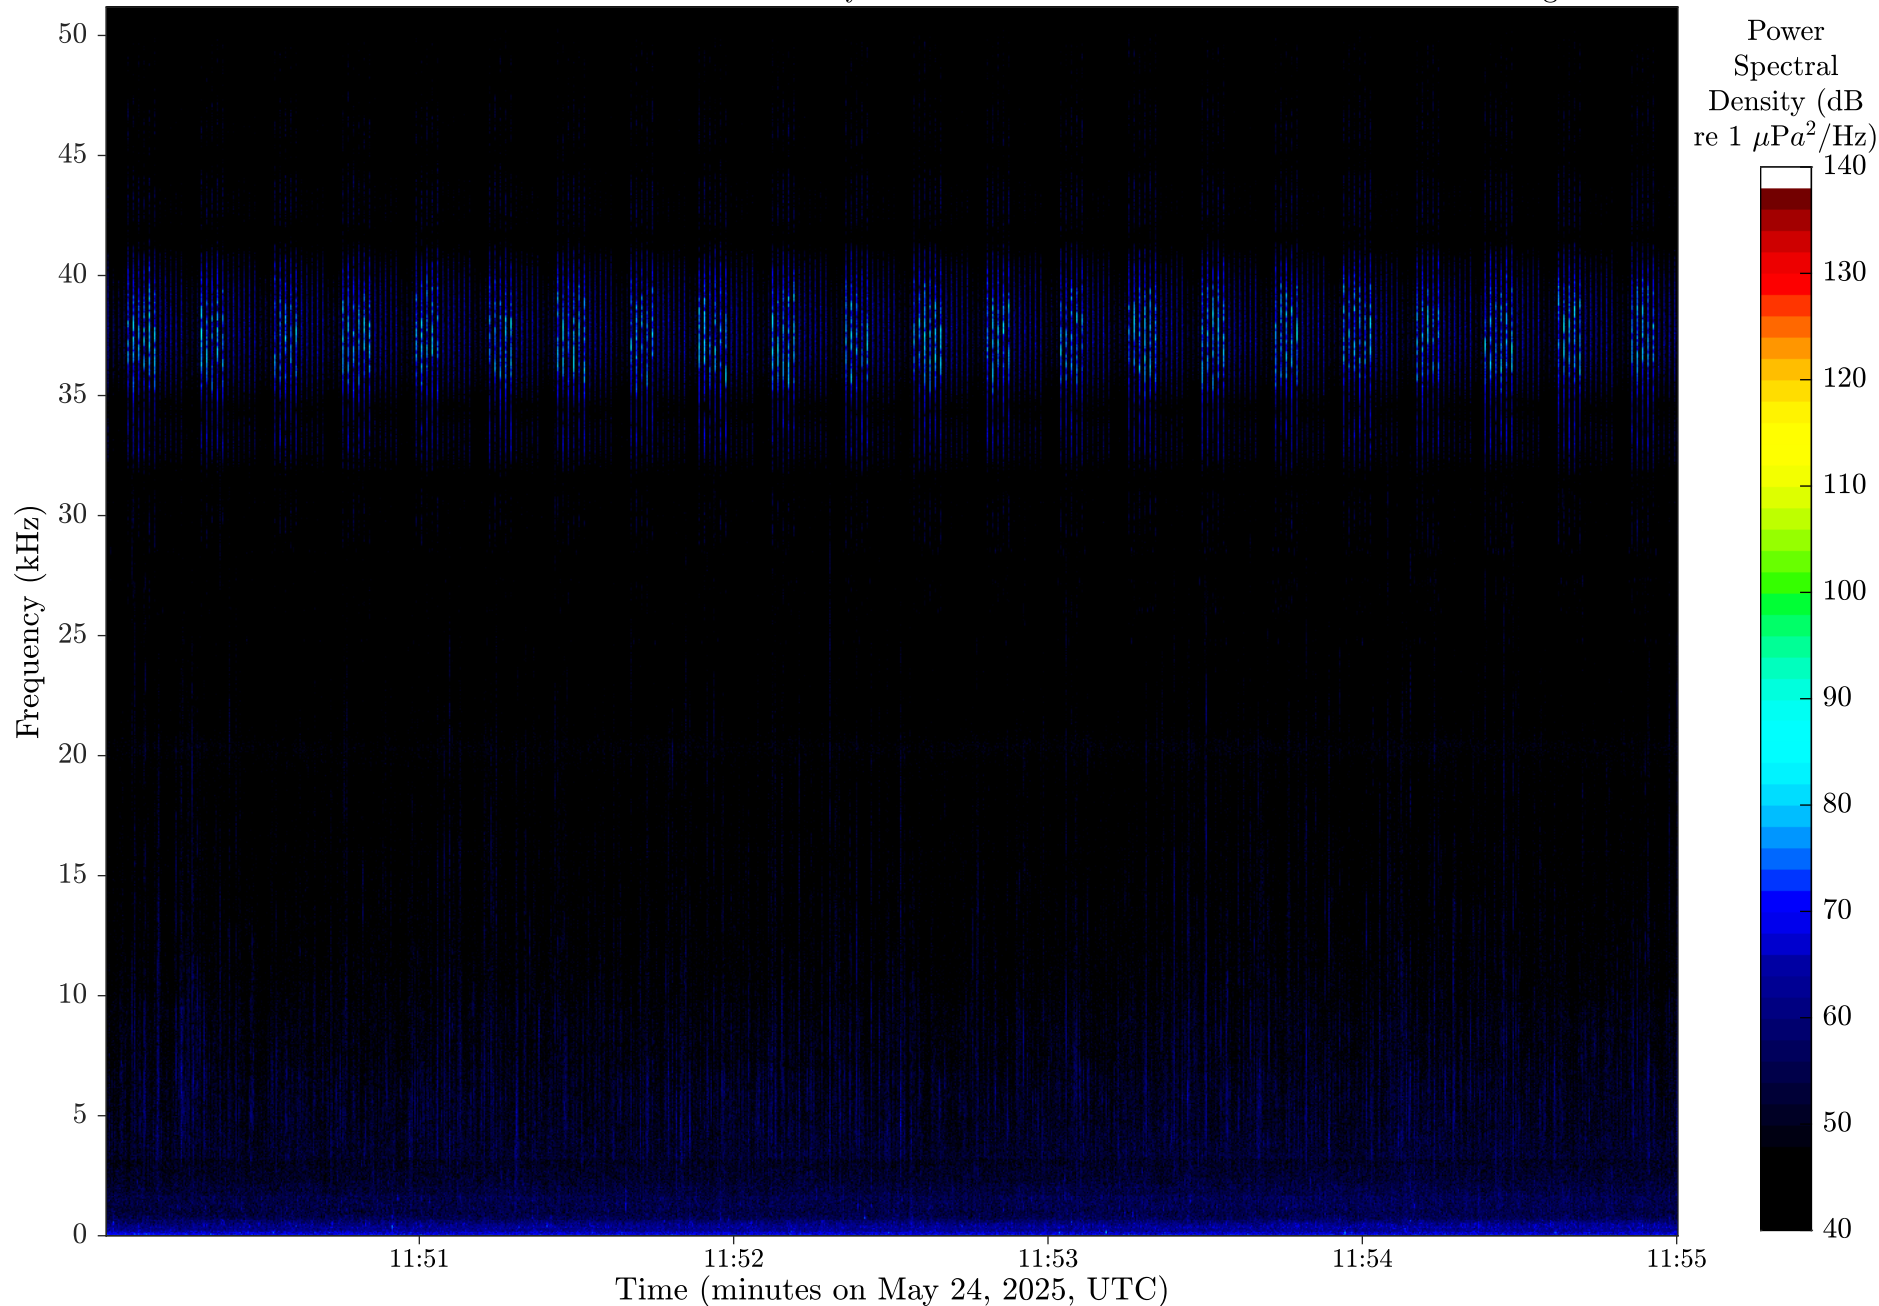


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:31 UTC

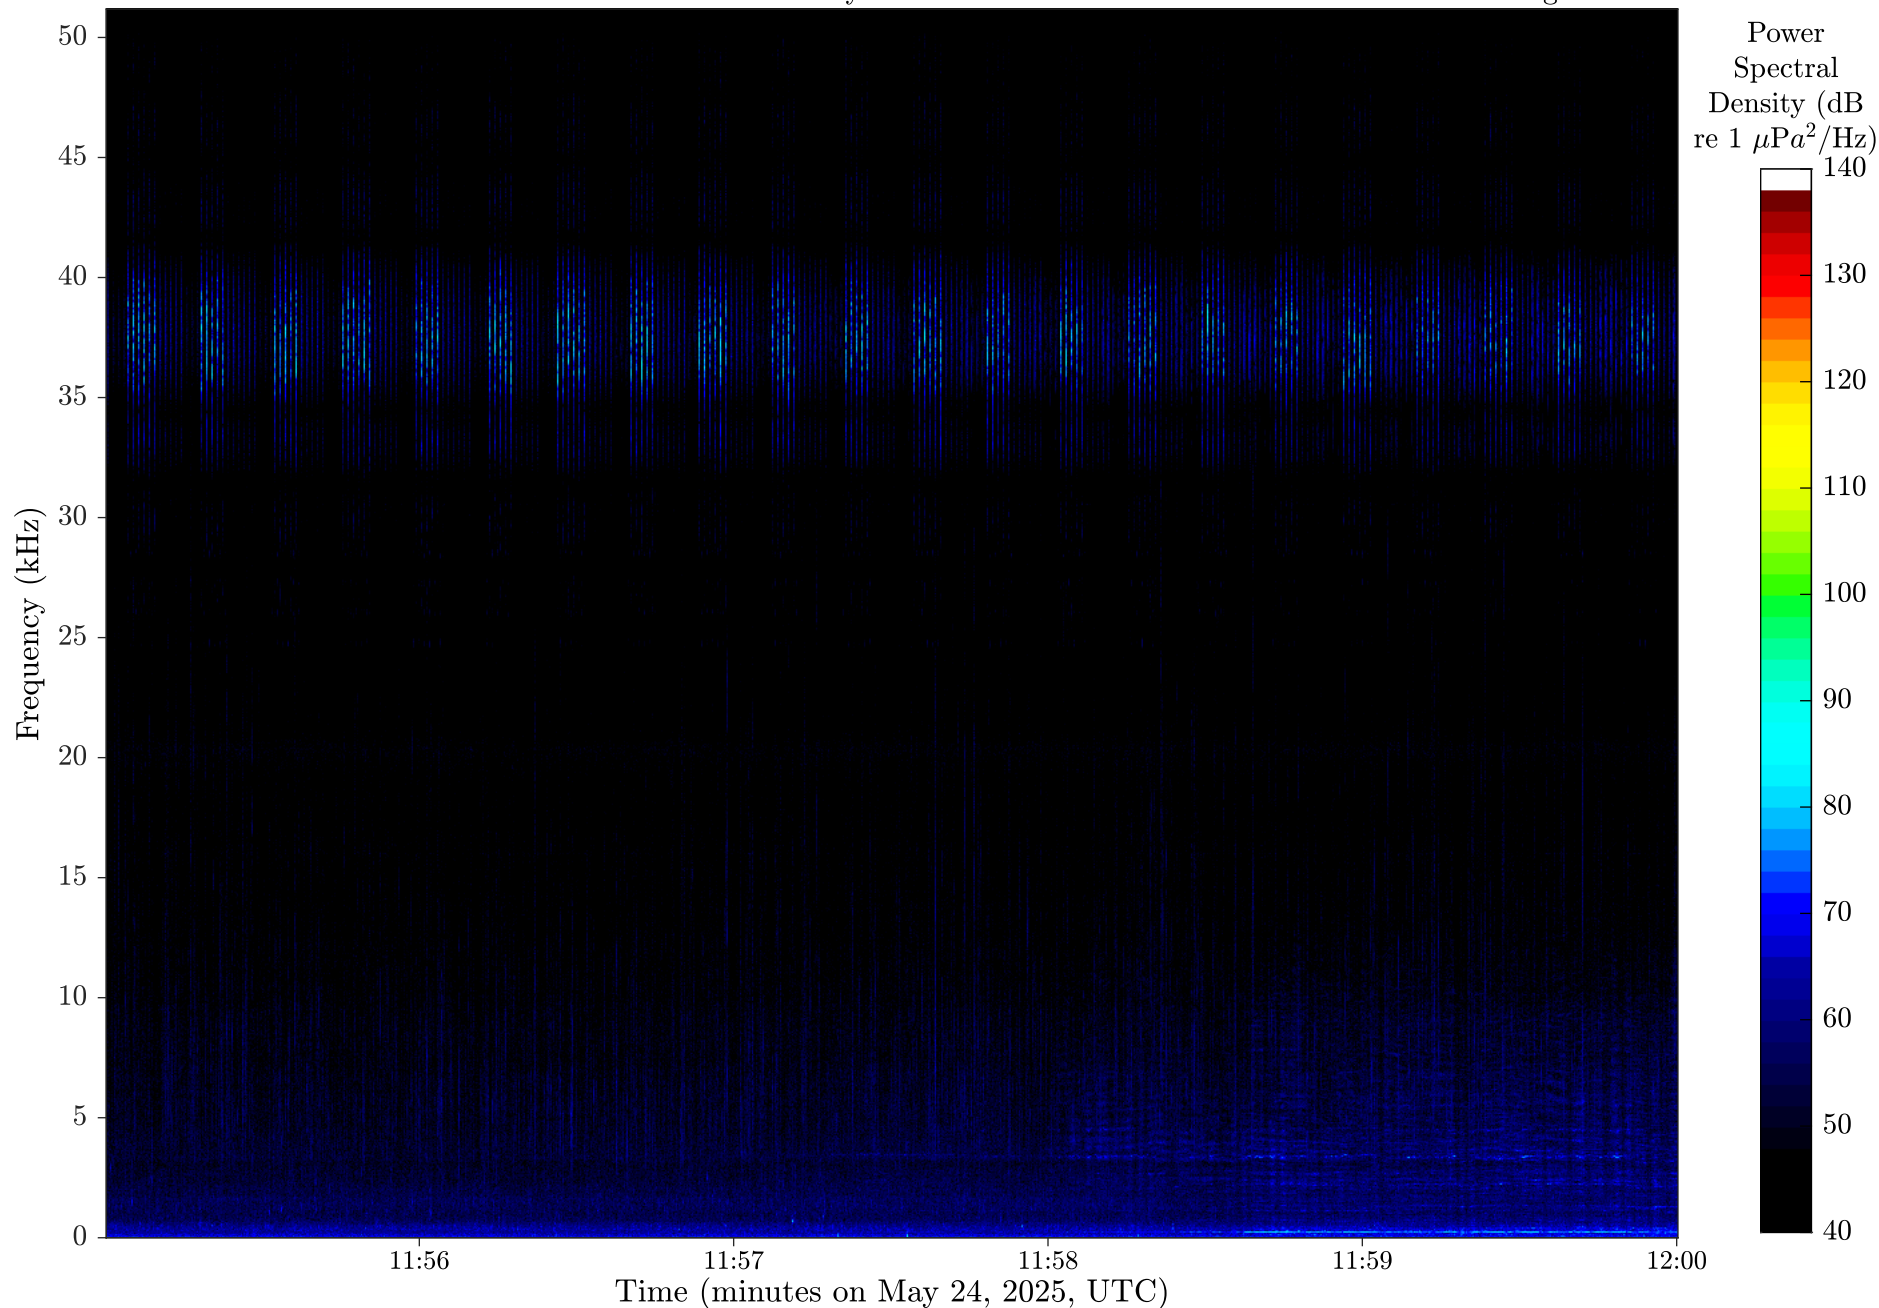


Comments: 31 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:38 UTC

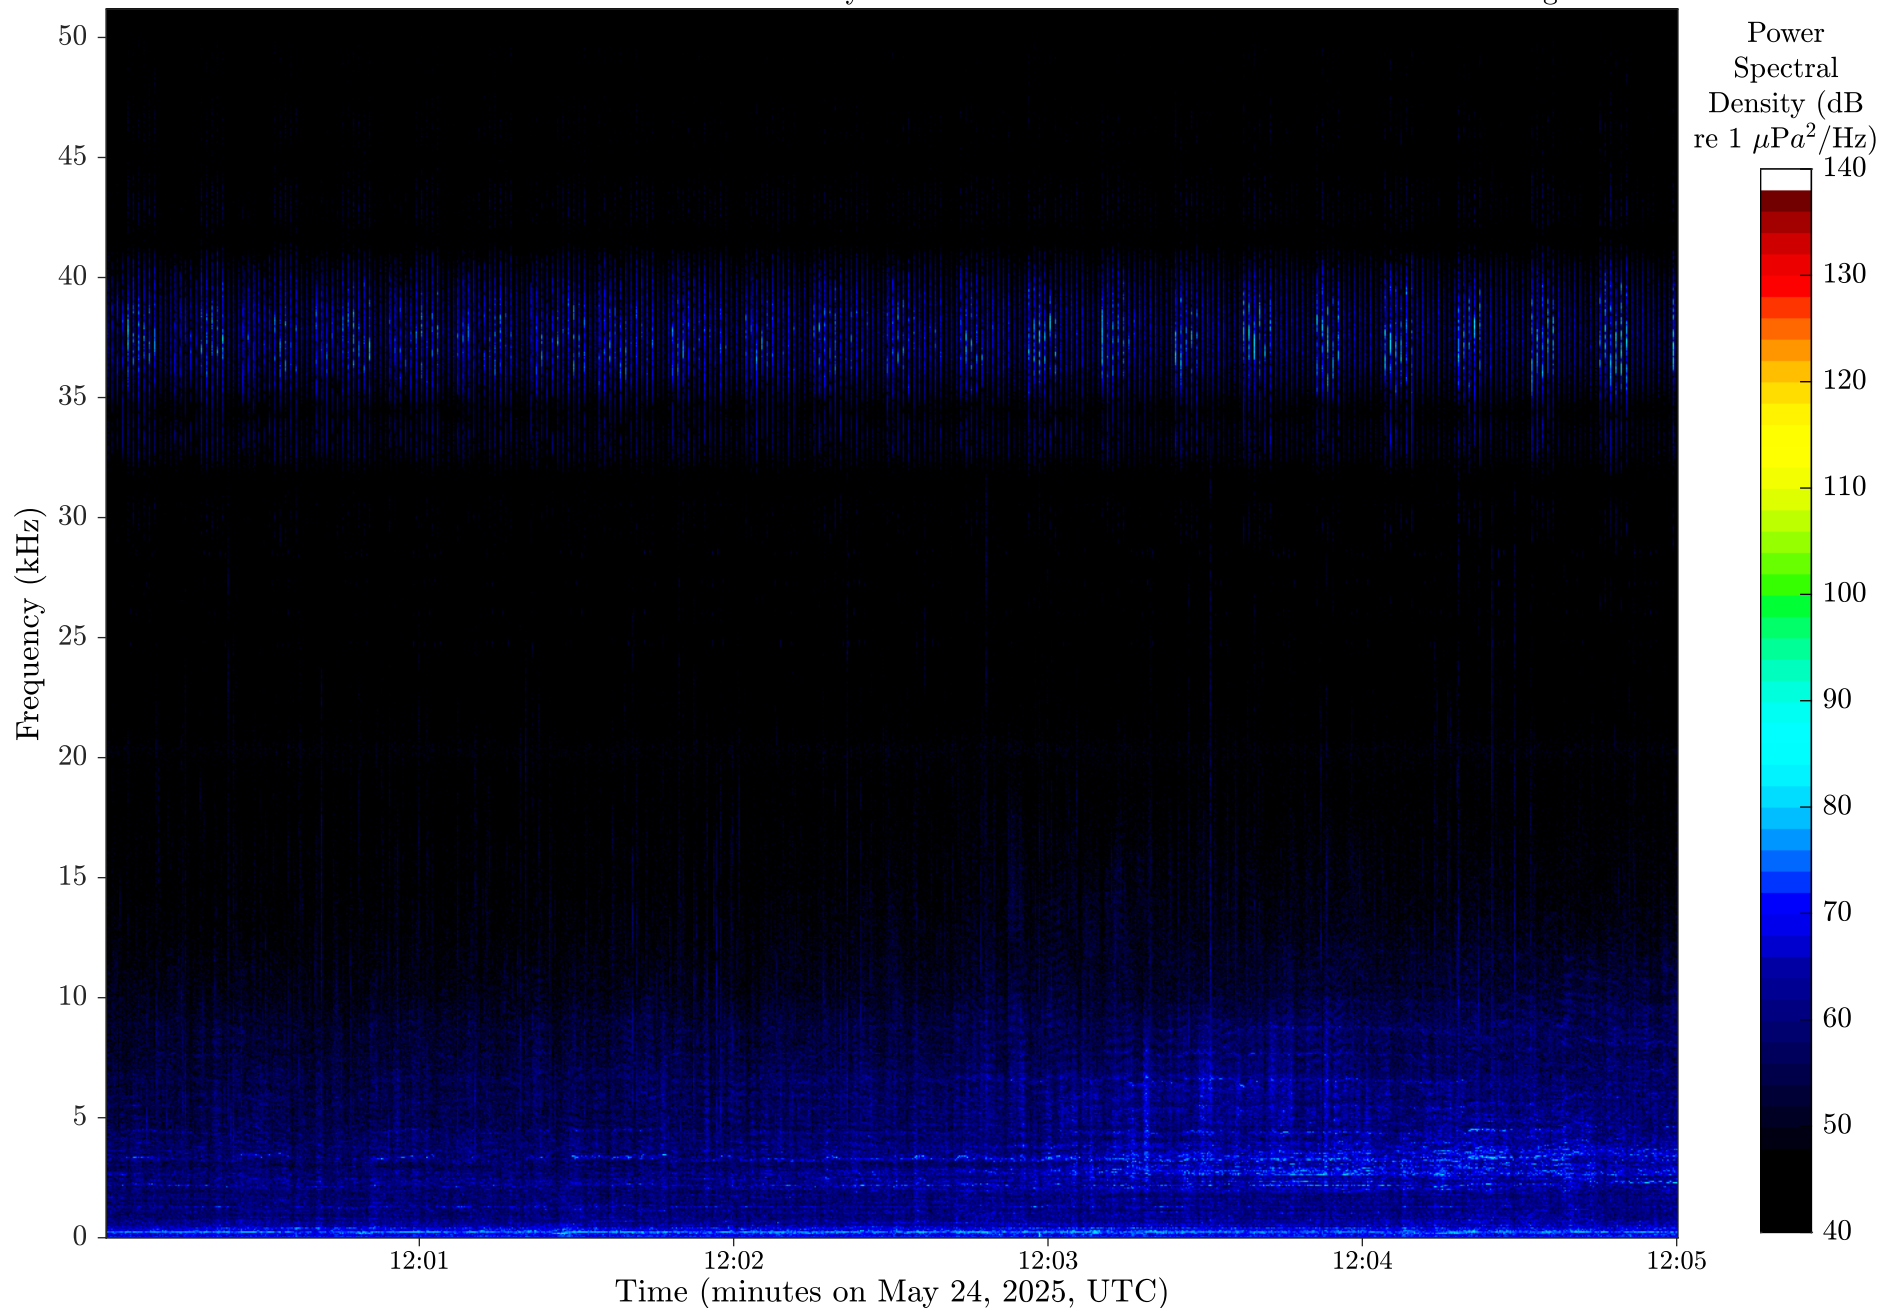


Comments: 28.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:46 UTC

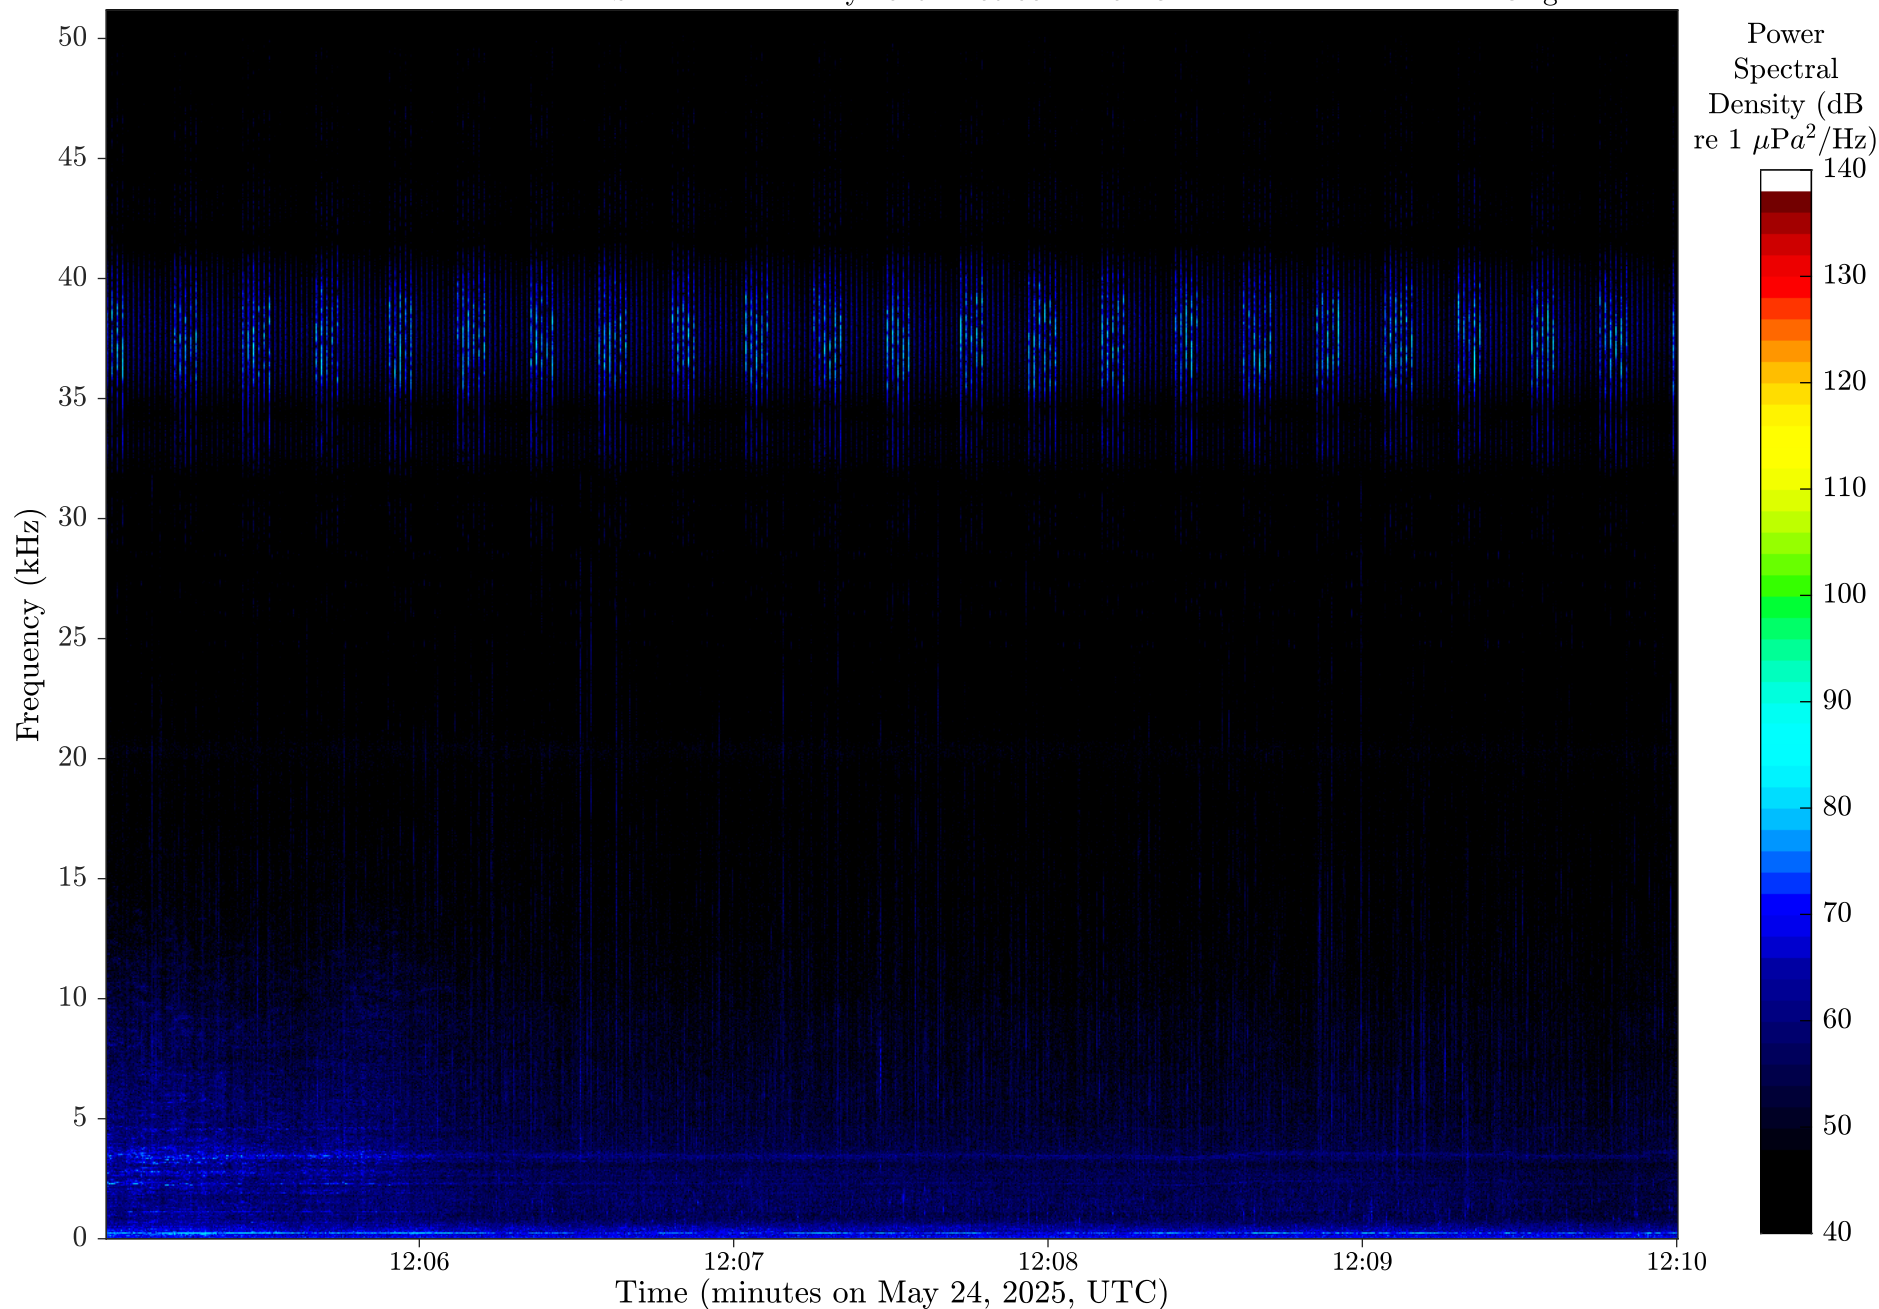


Comments: 29.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:53 UTC

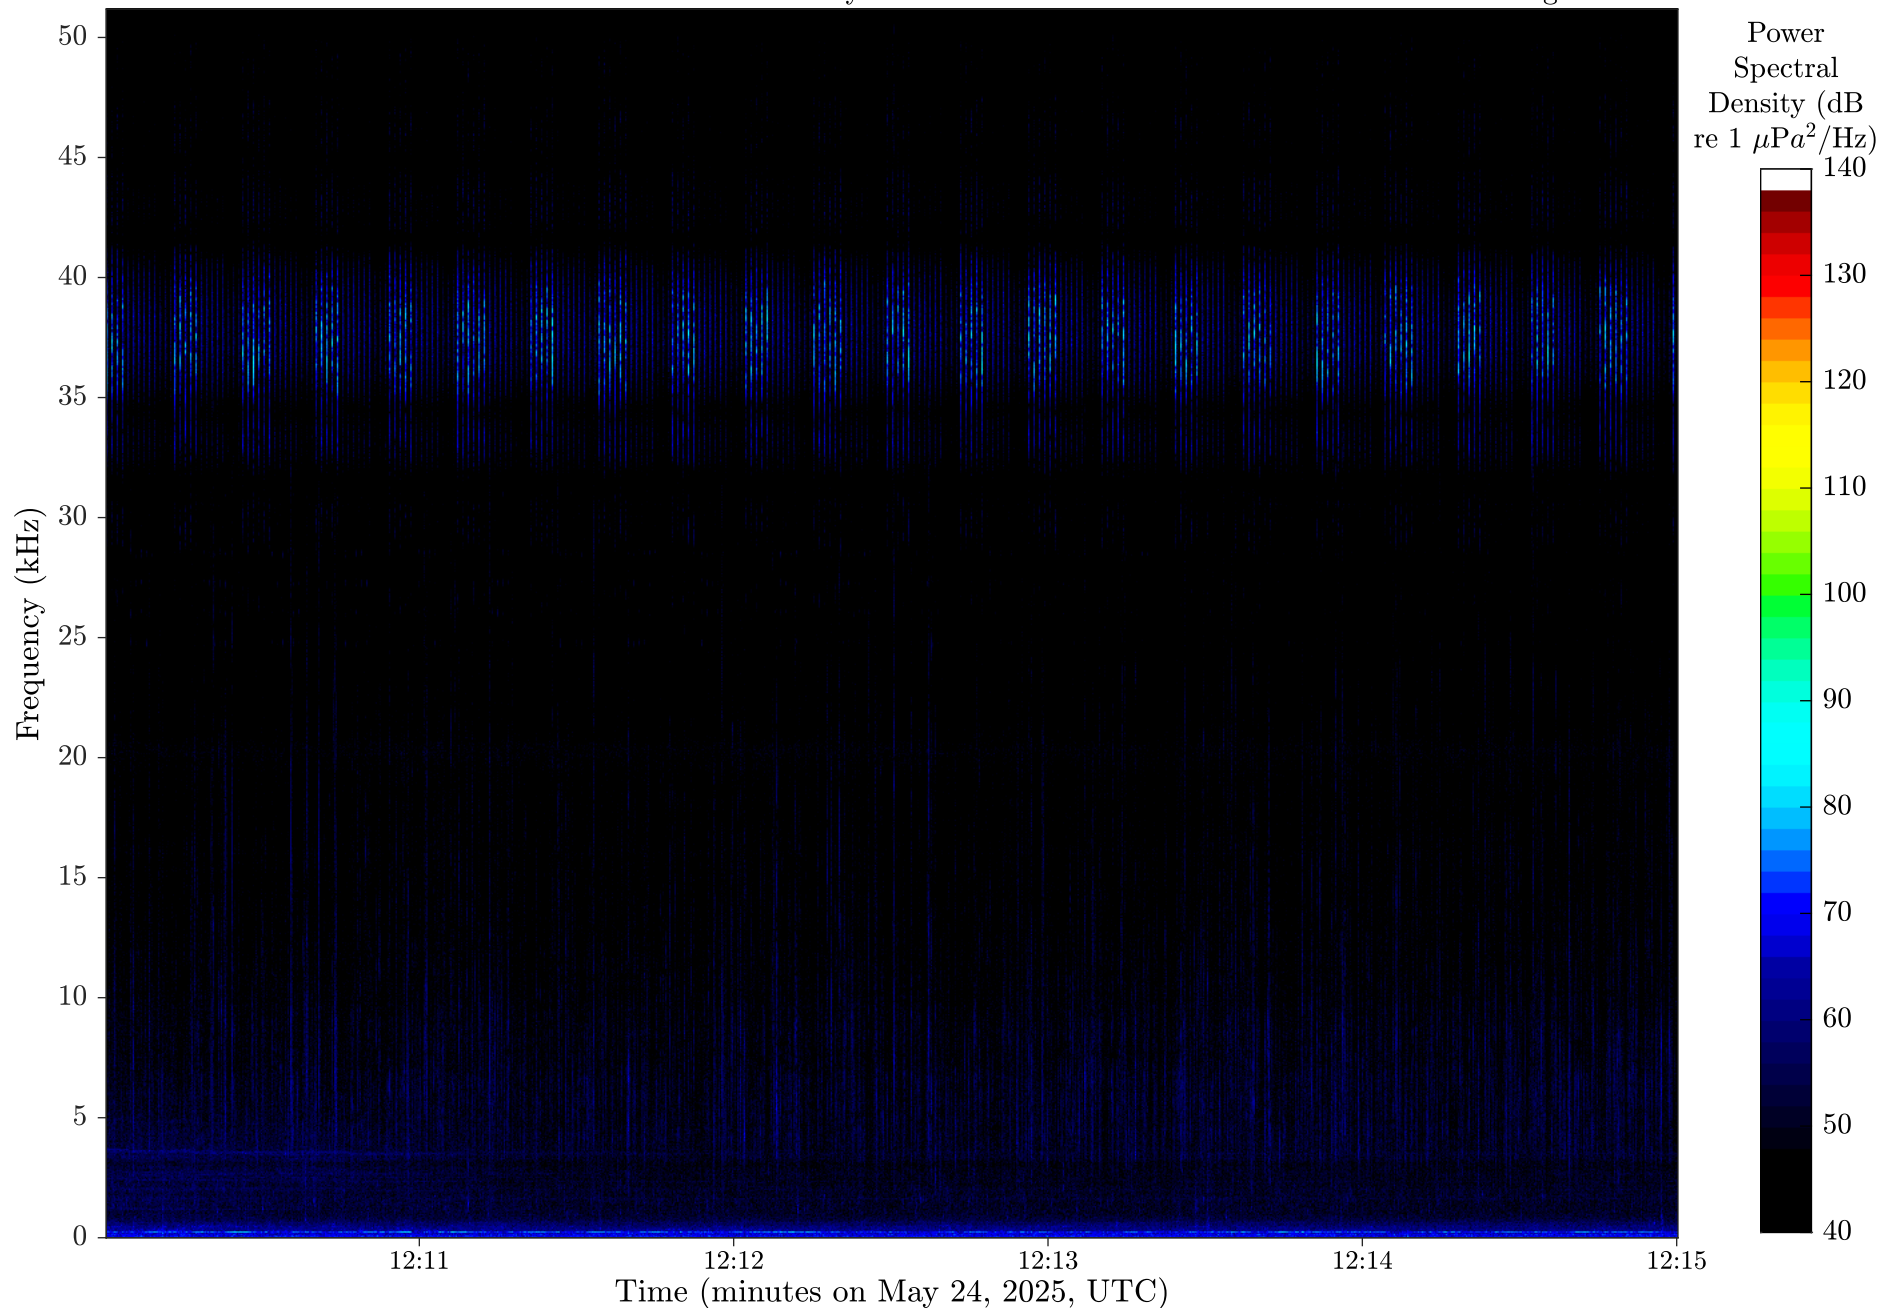


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:30:01 UTC

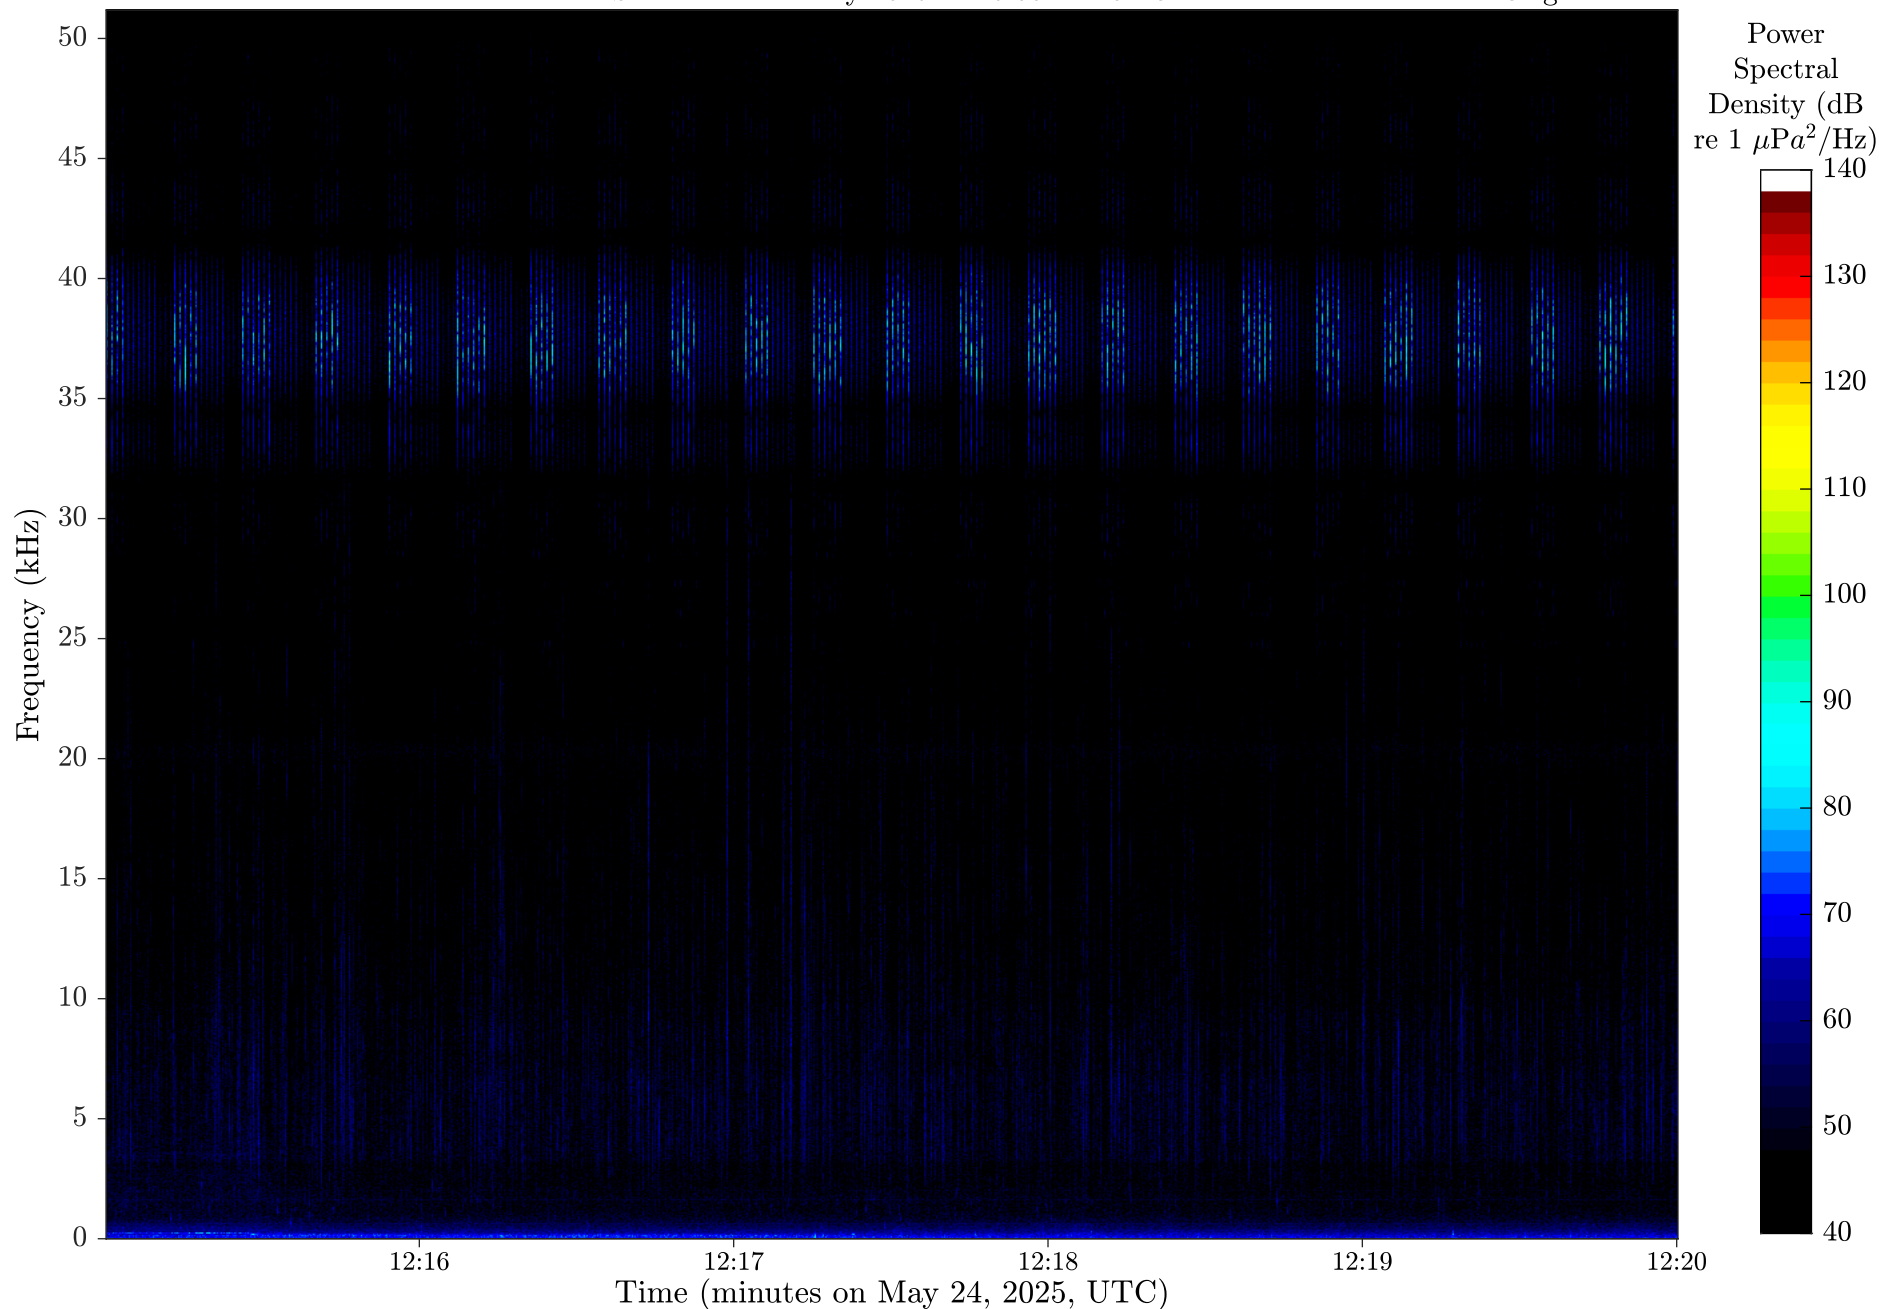


Comments: 32.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:30:08 UTC

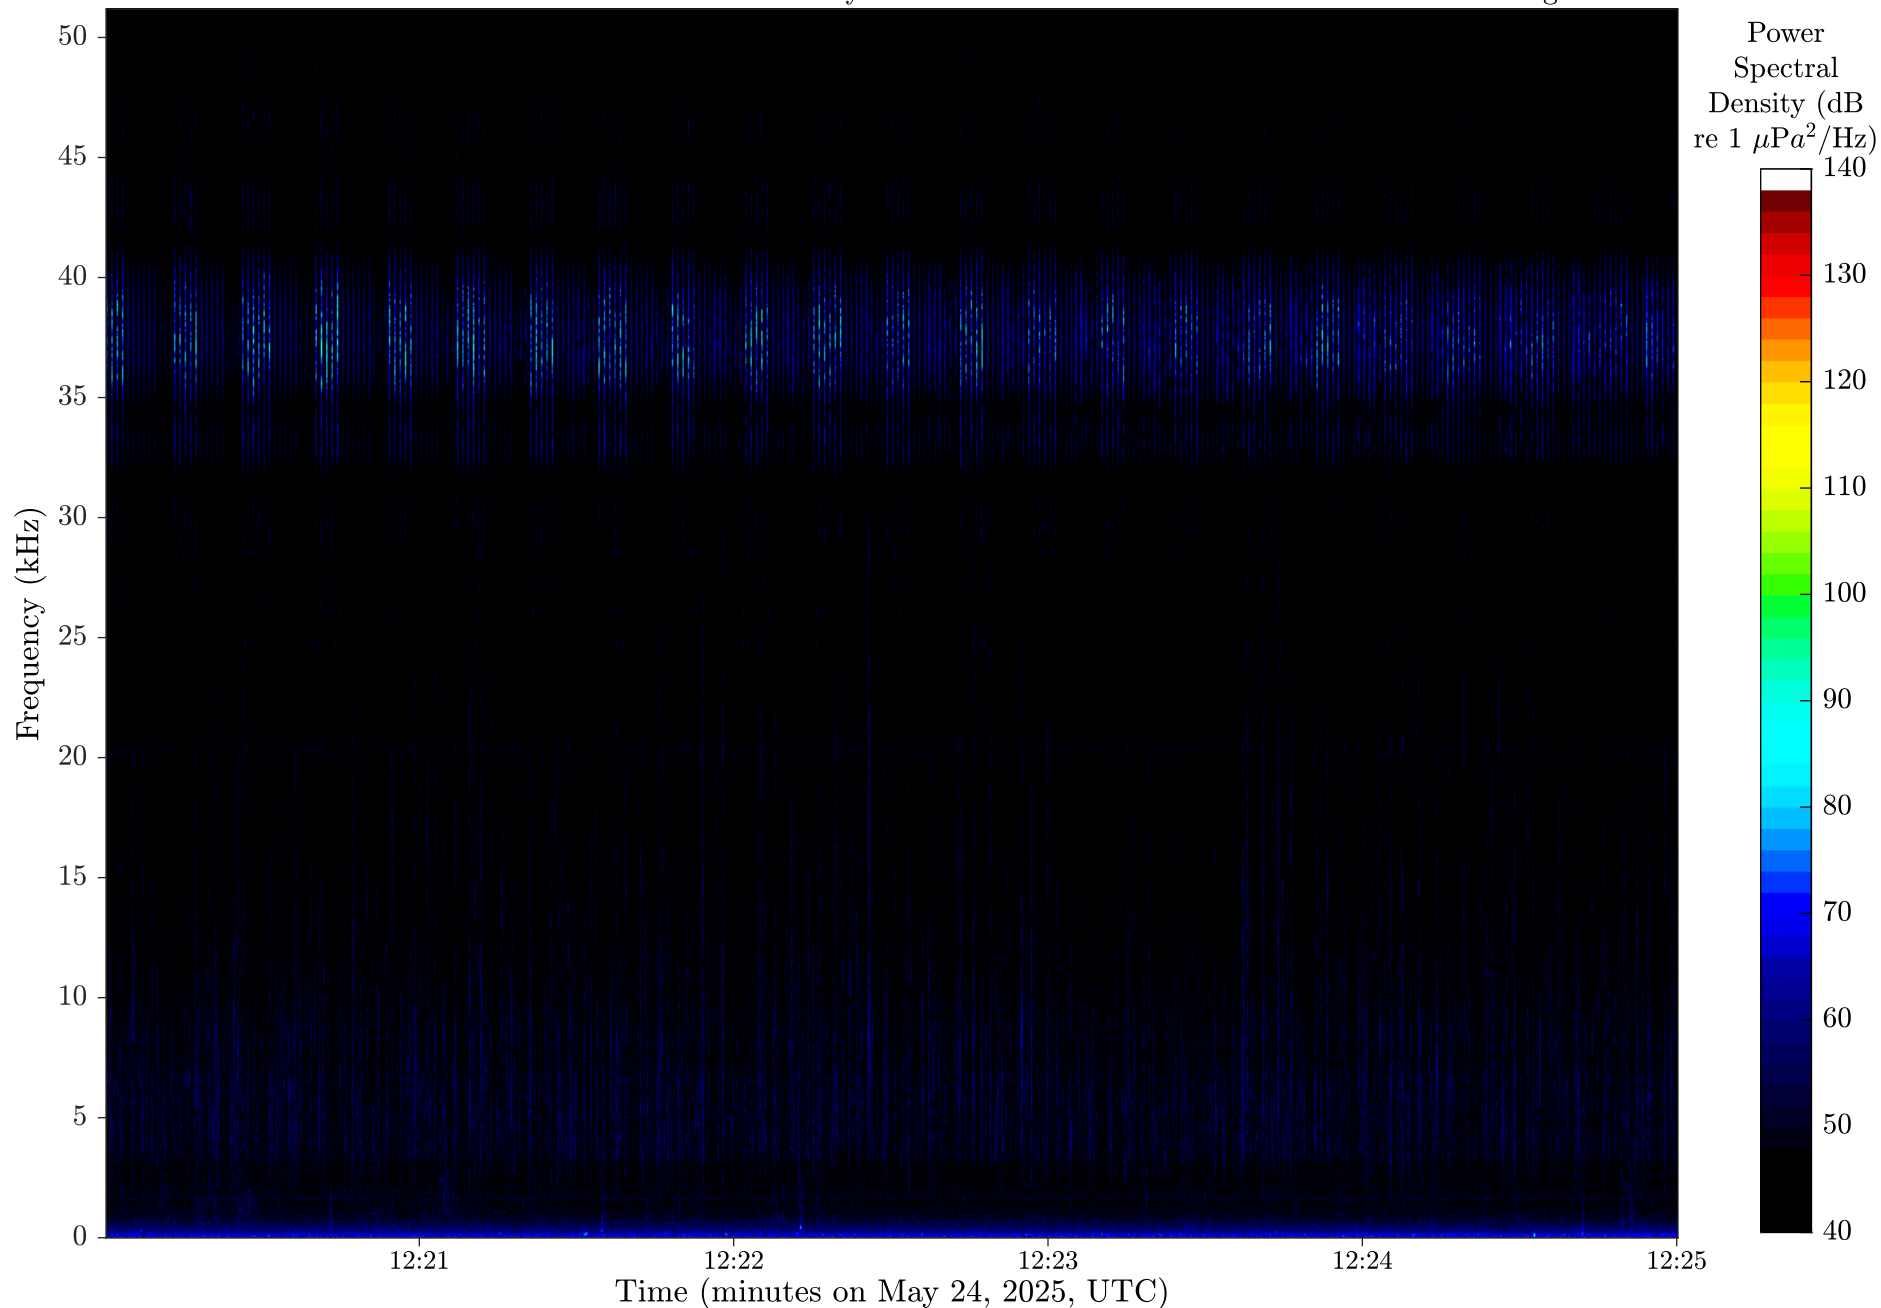


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:30:16 UTC

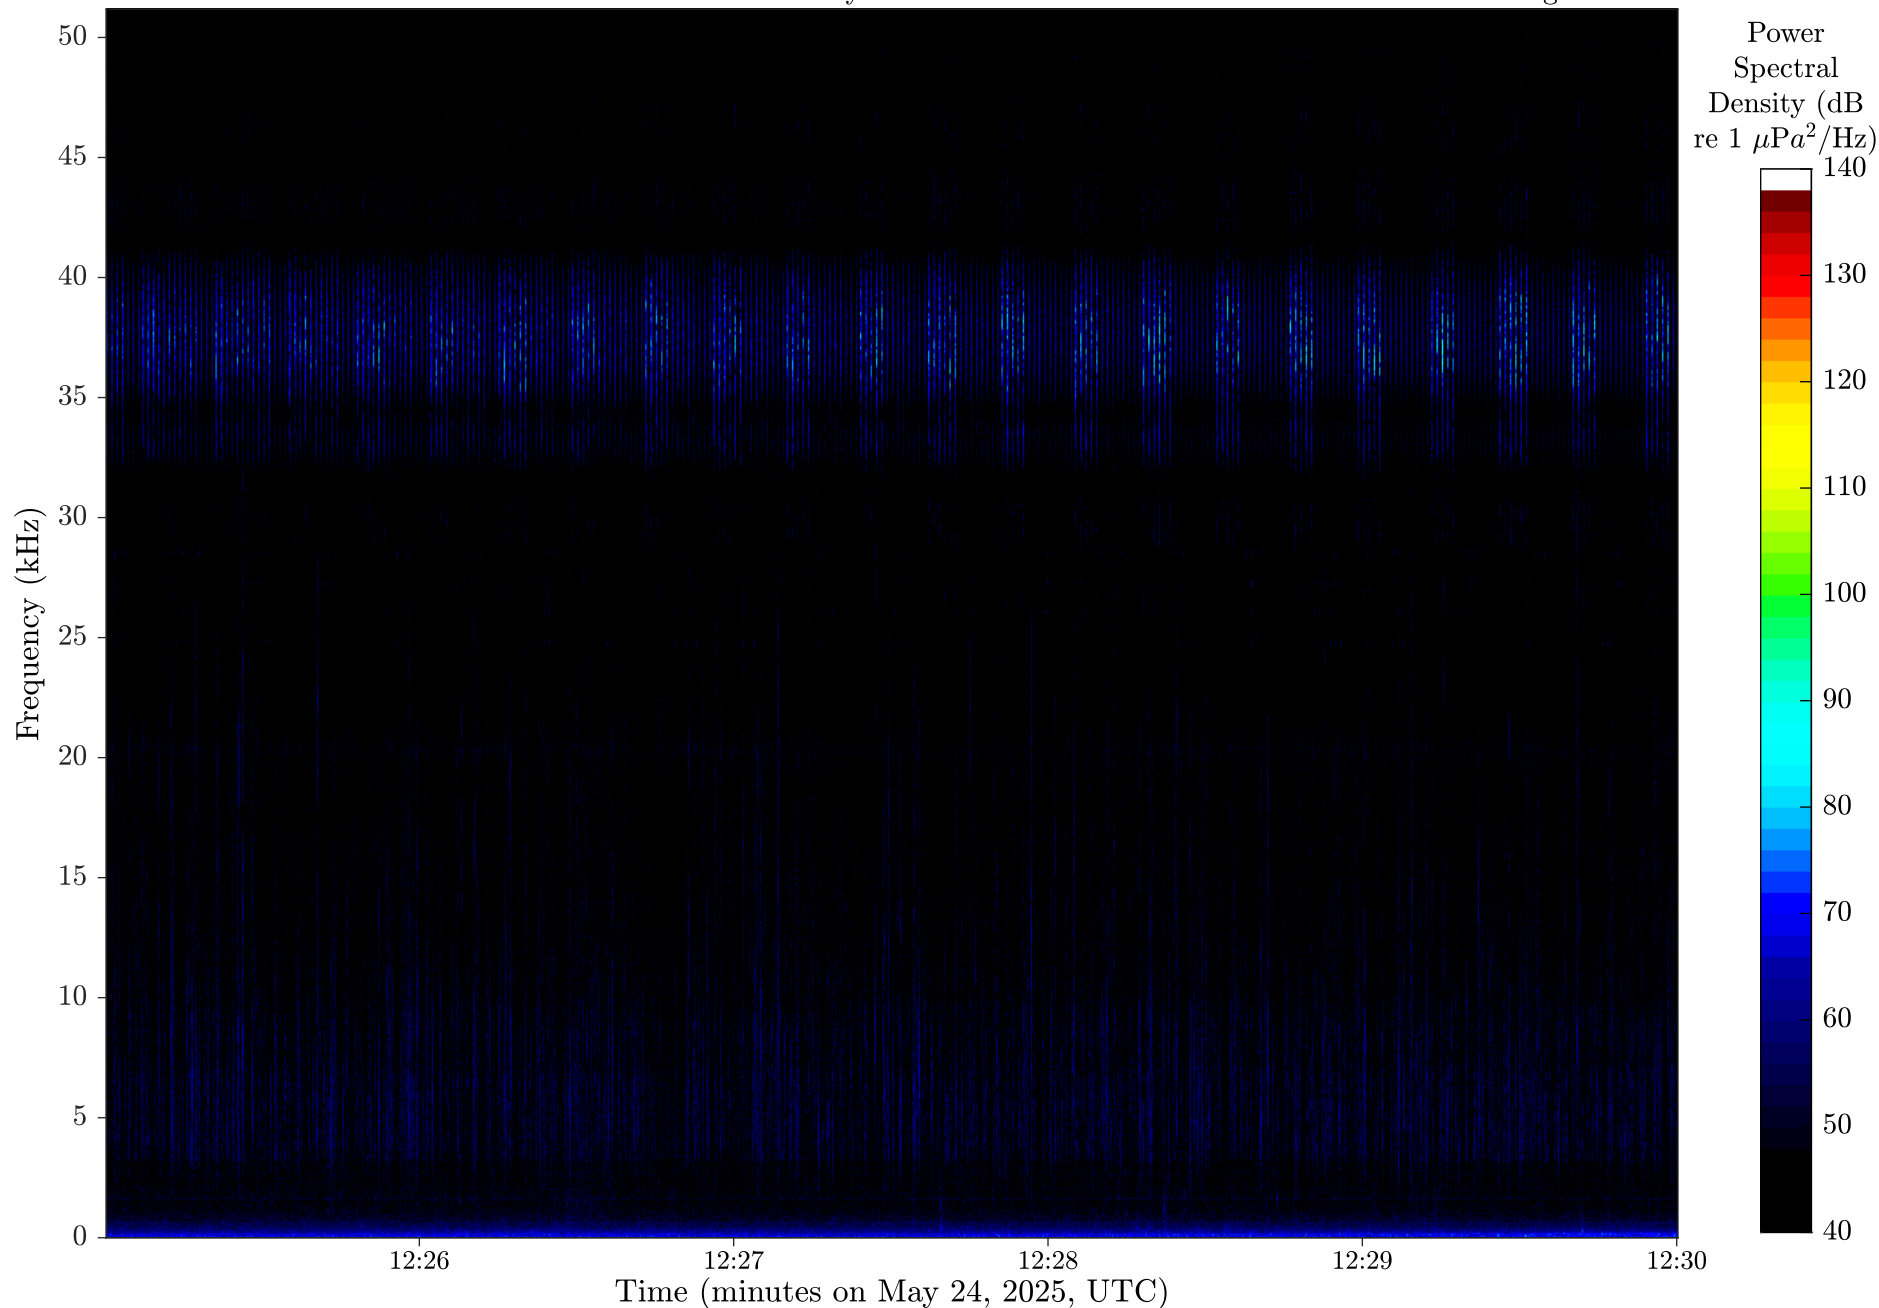

Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:30:23 UTC

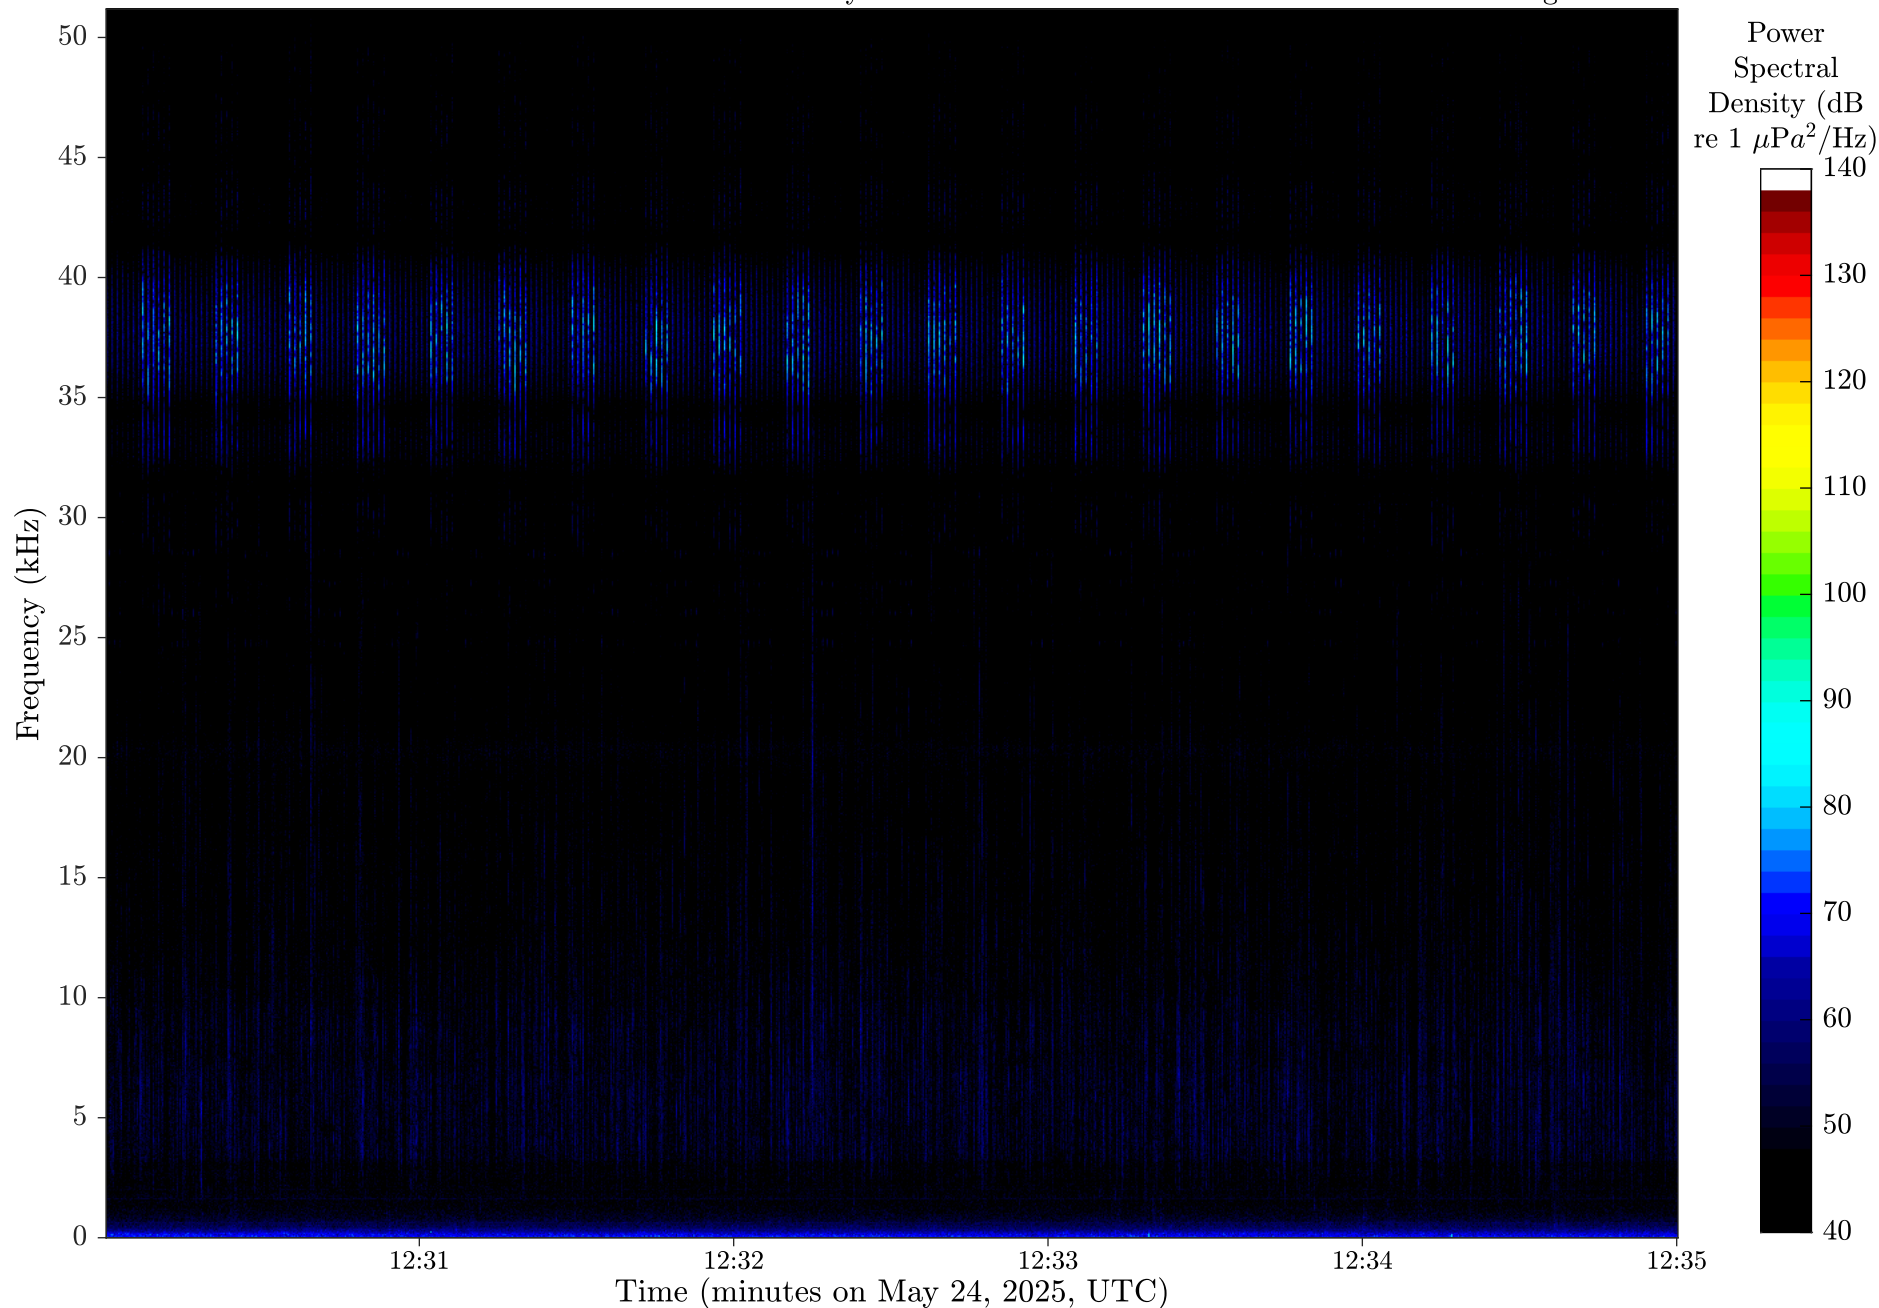

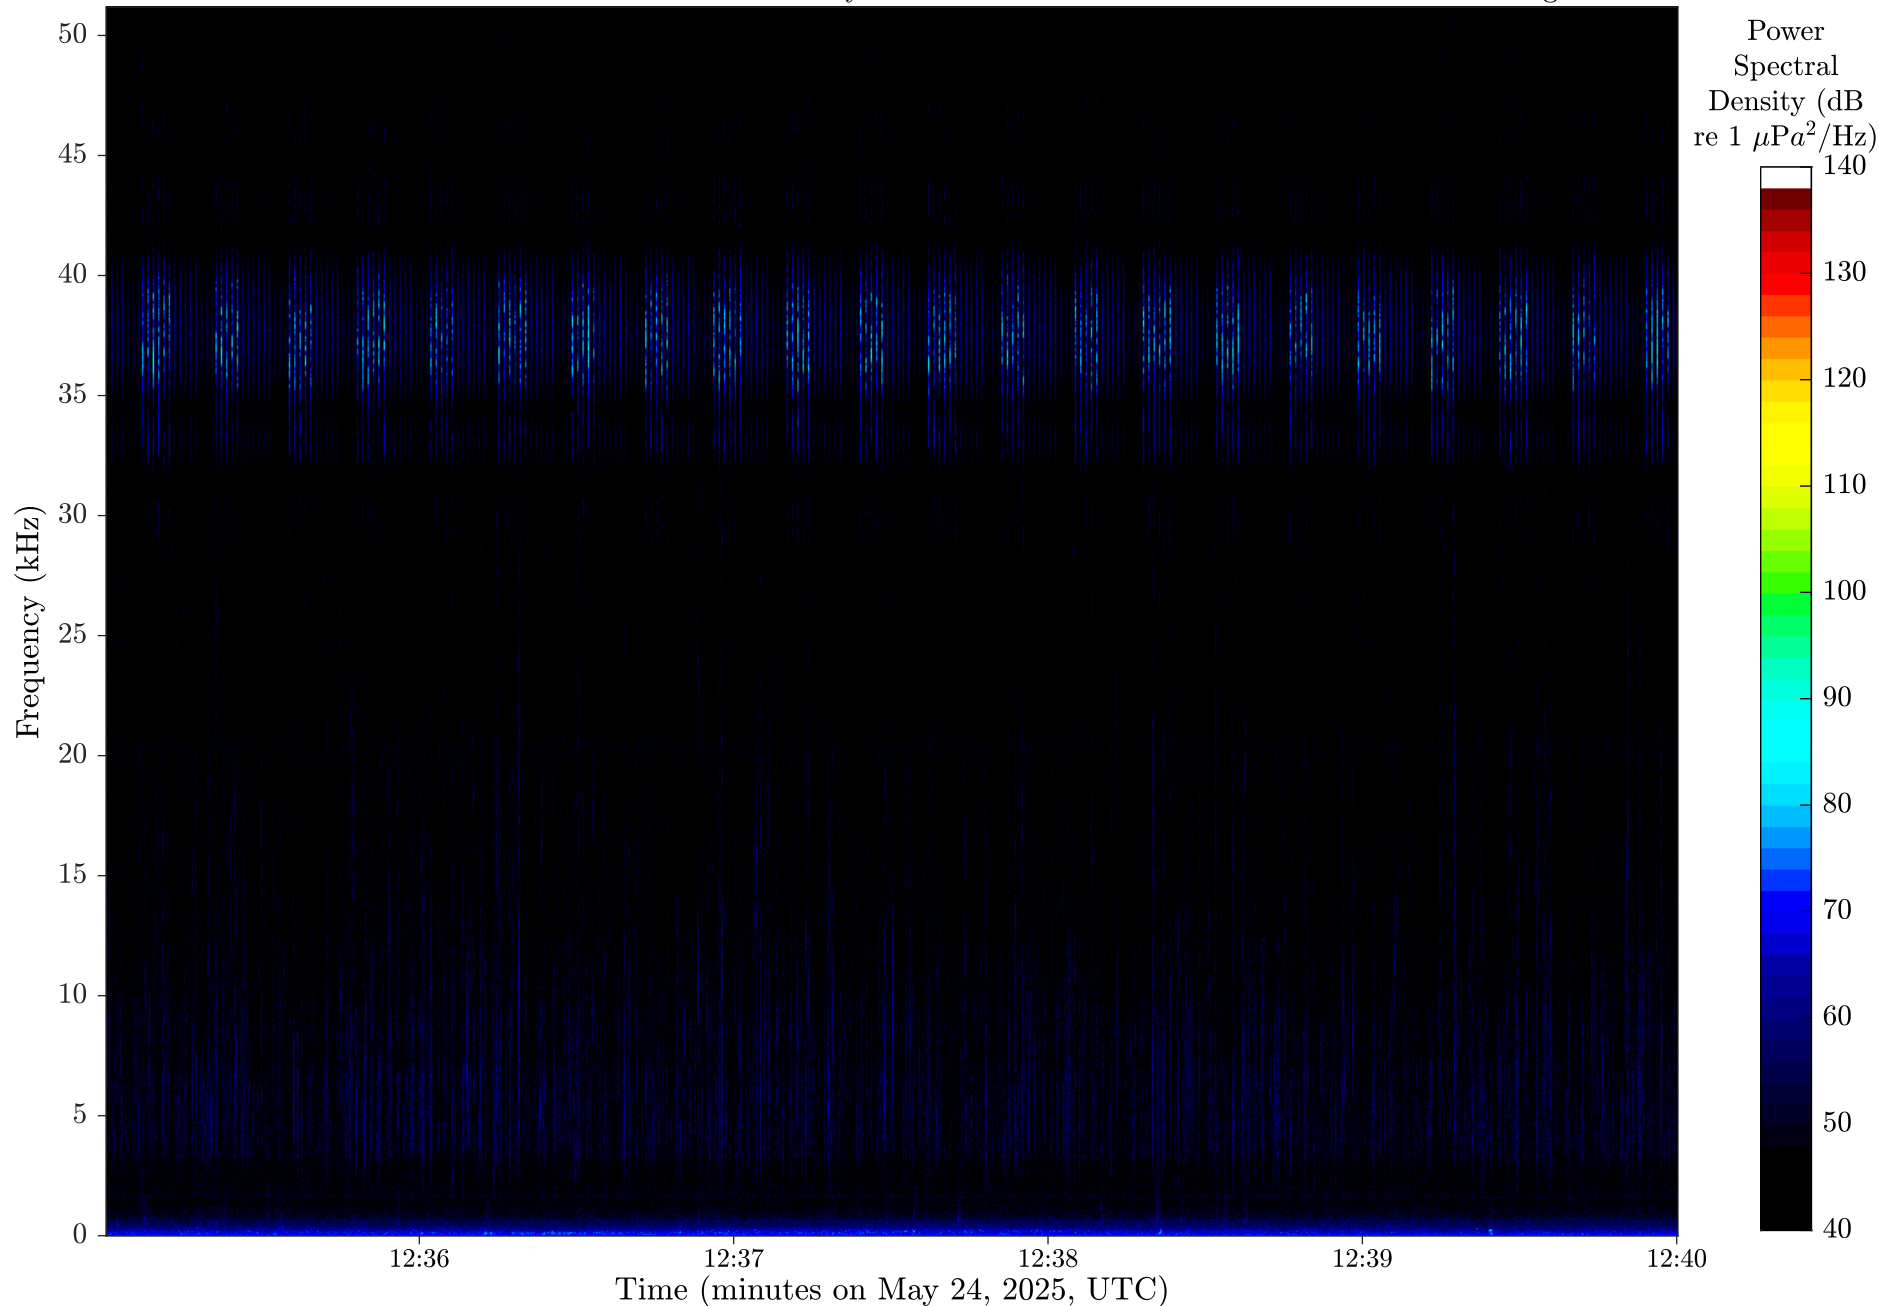


Comments: 32.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:30:38 UTC

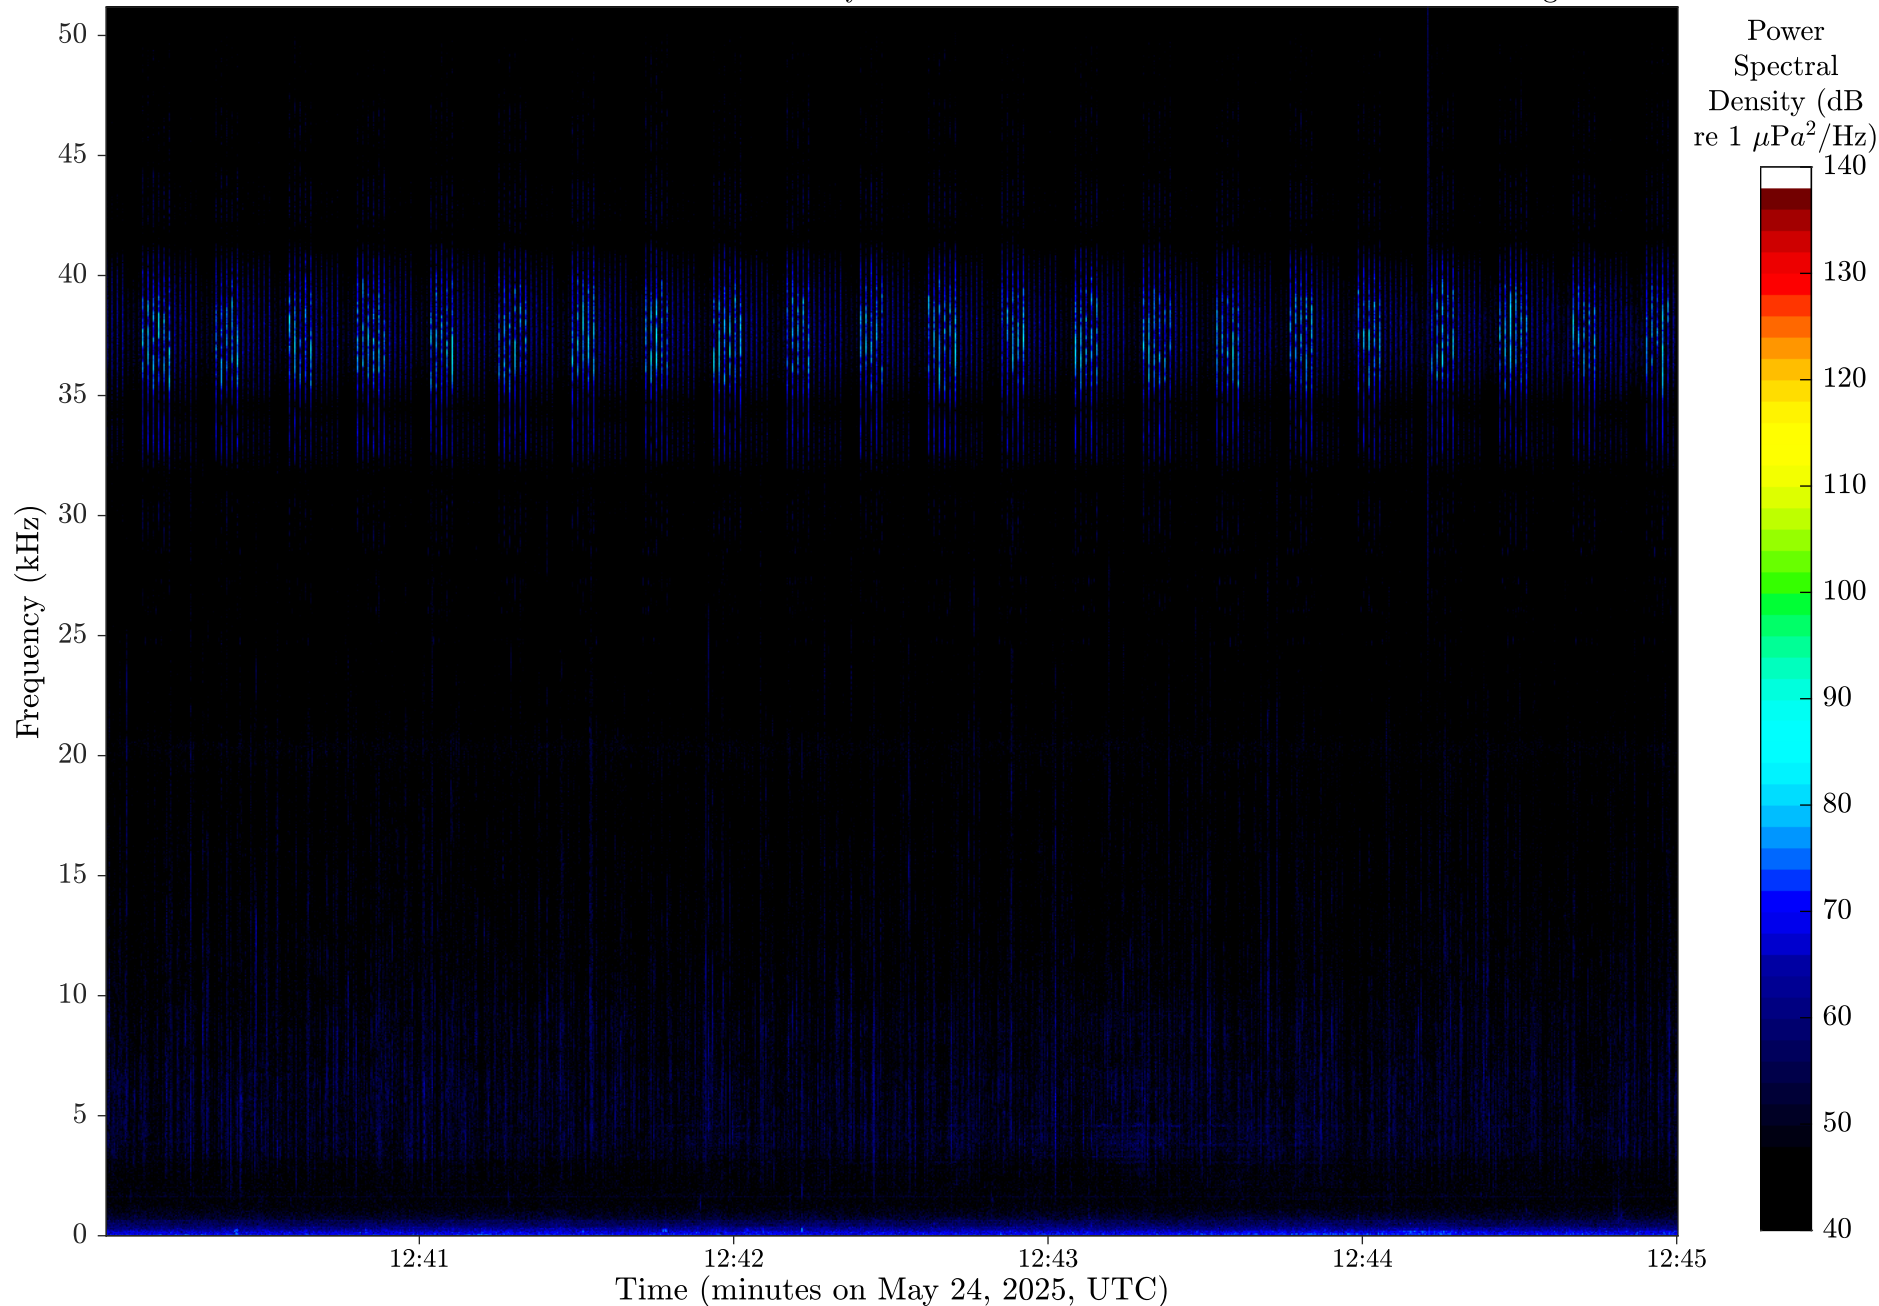


Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:30:46 UTC

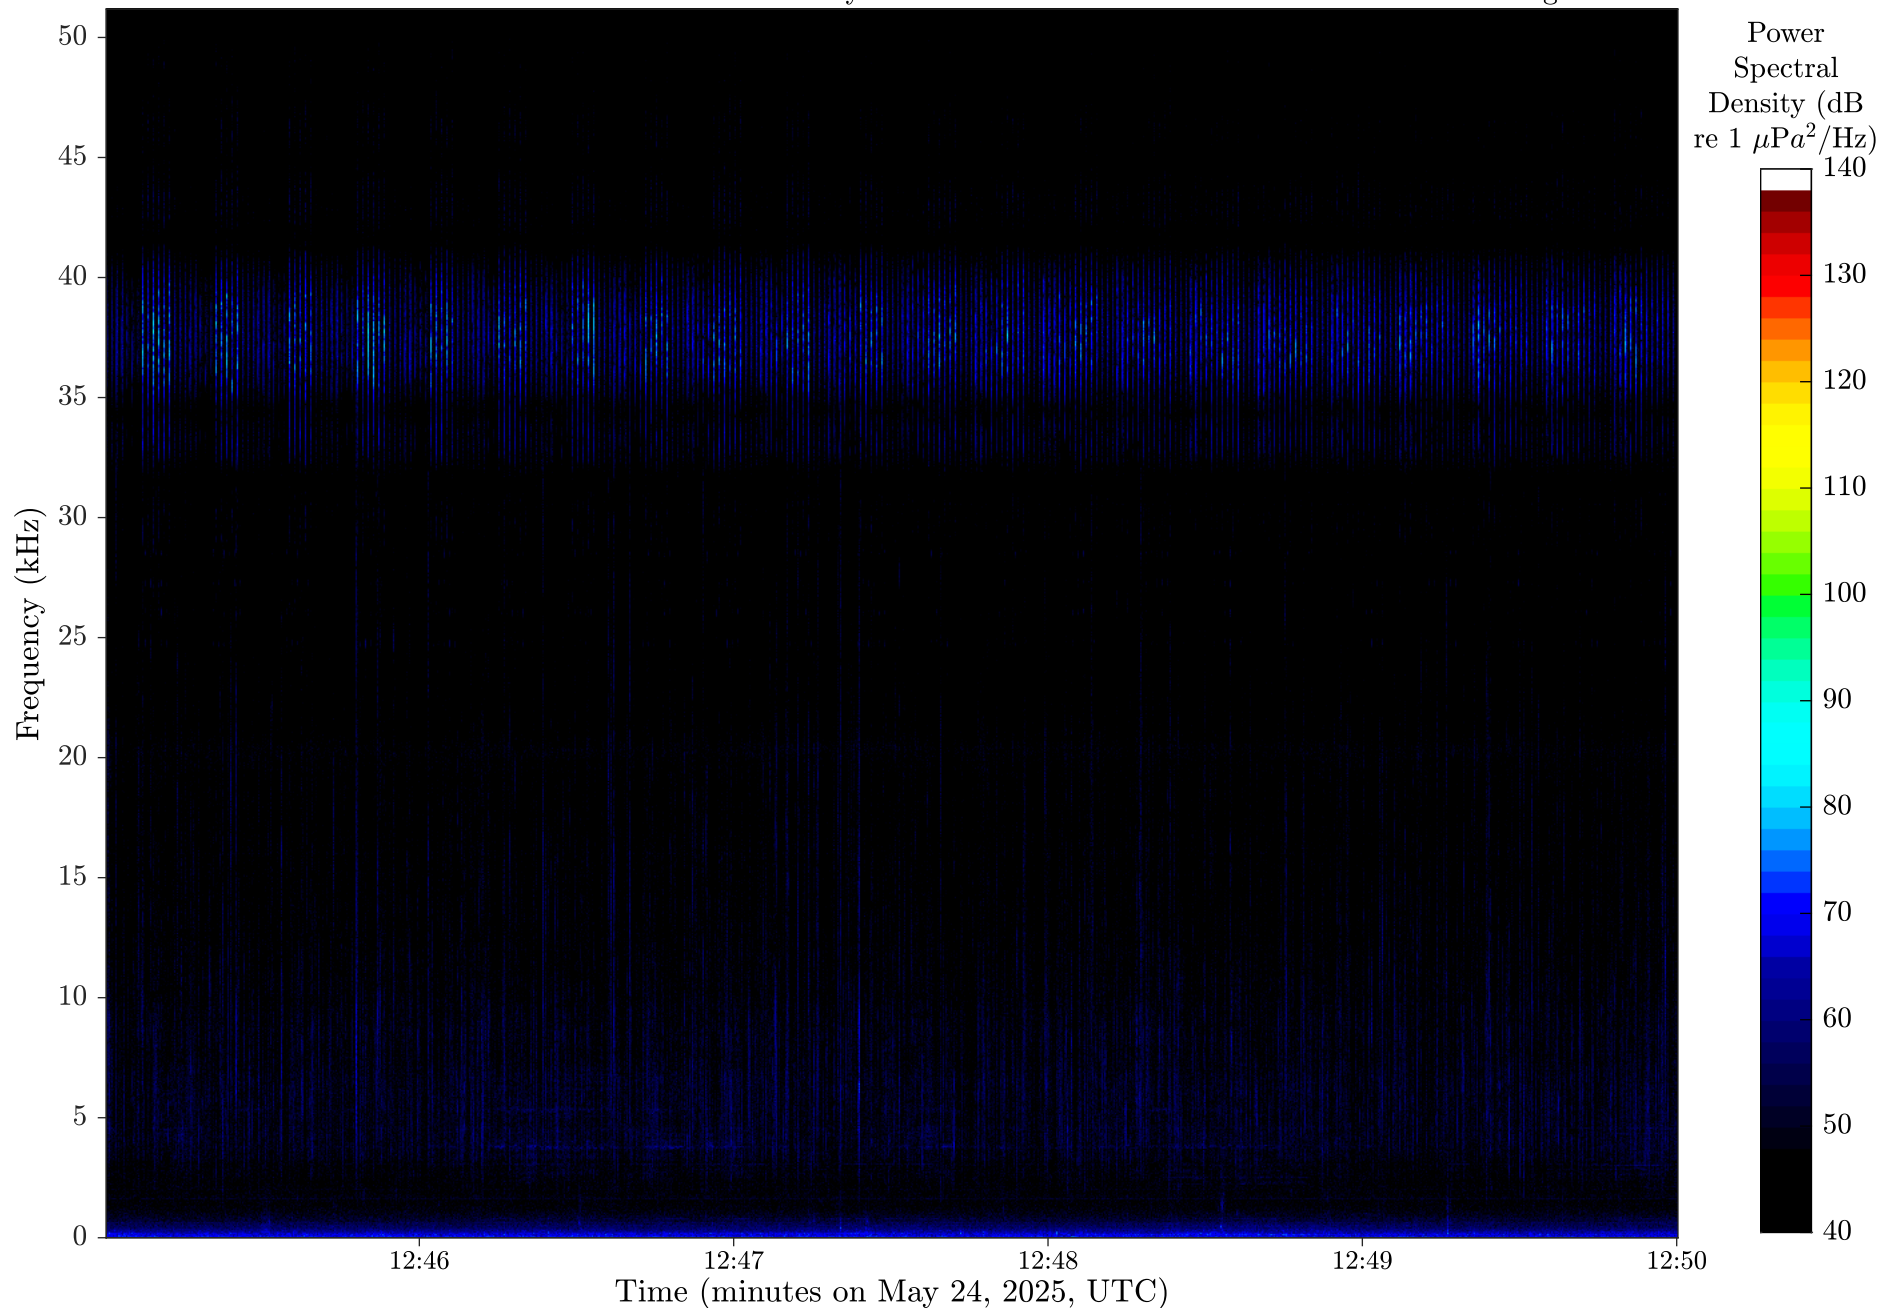


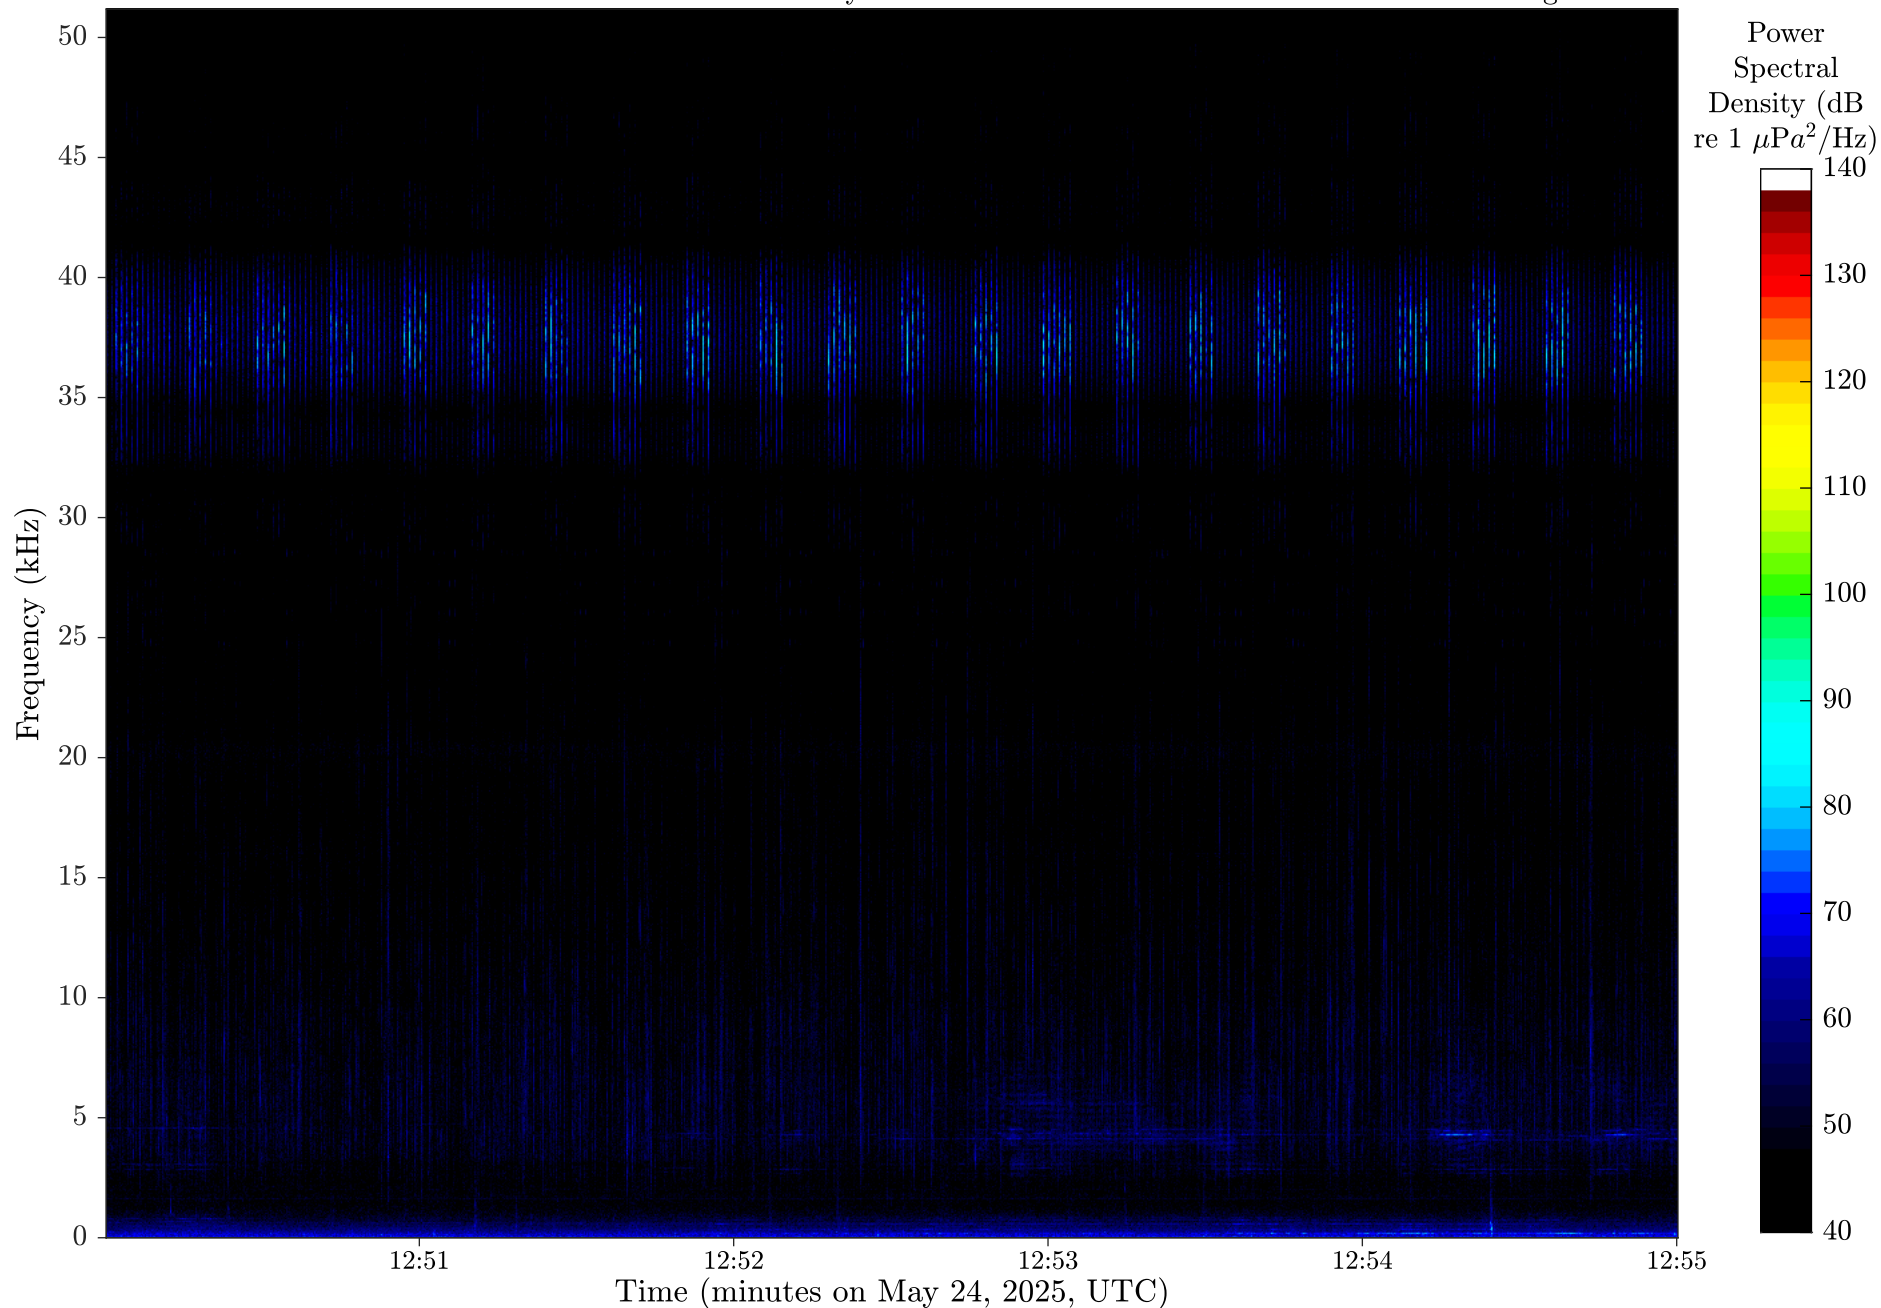


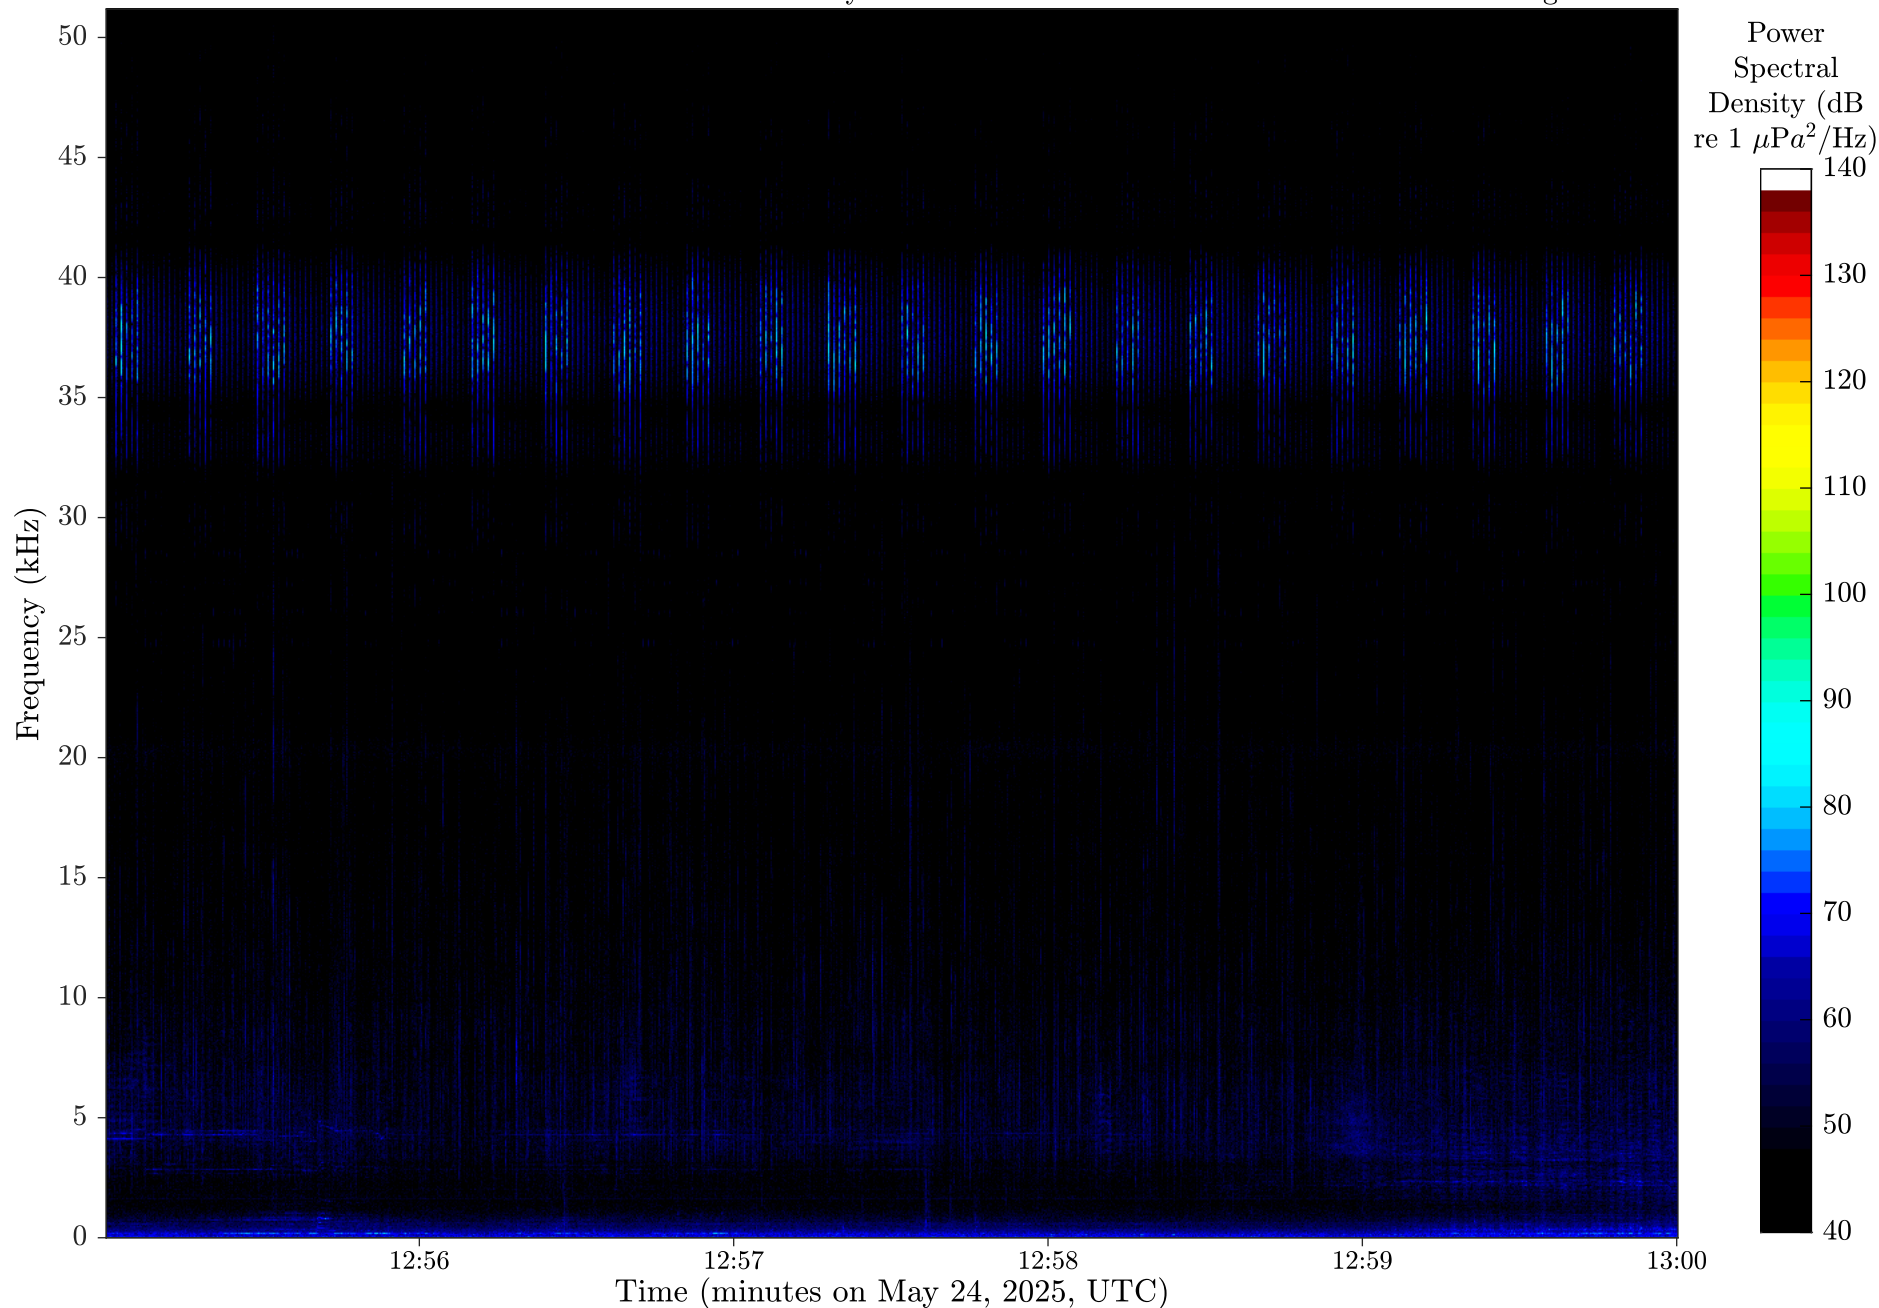

Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:31:08 UTC

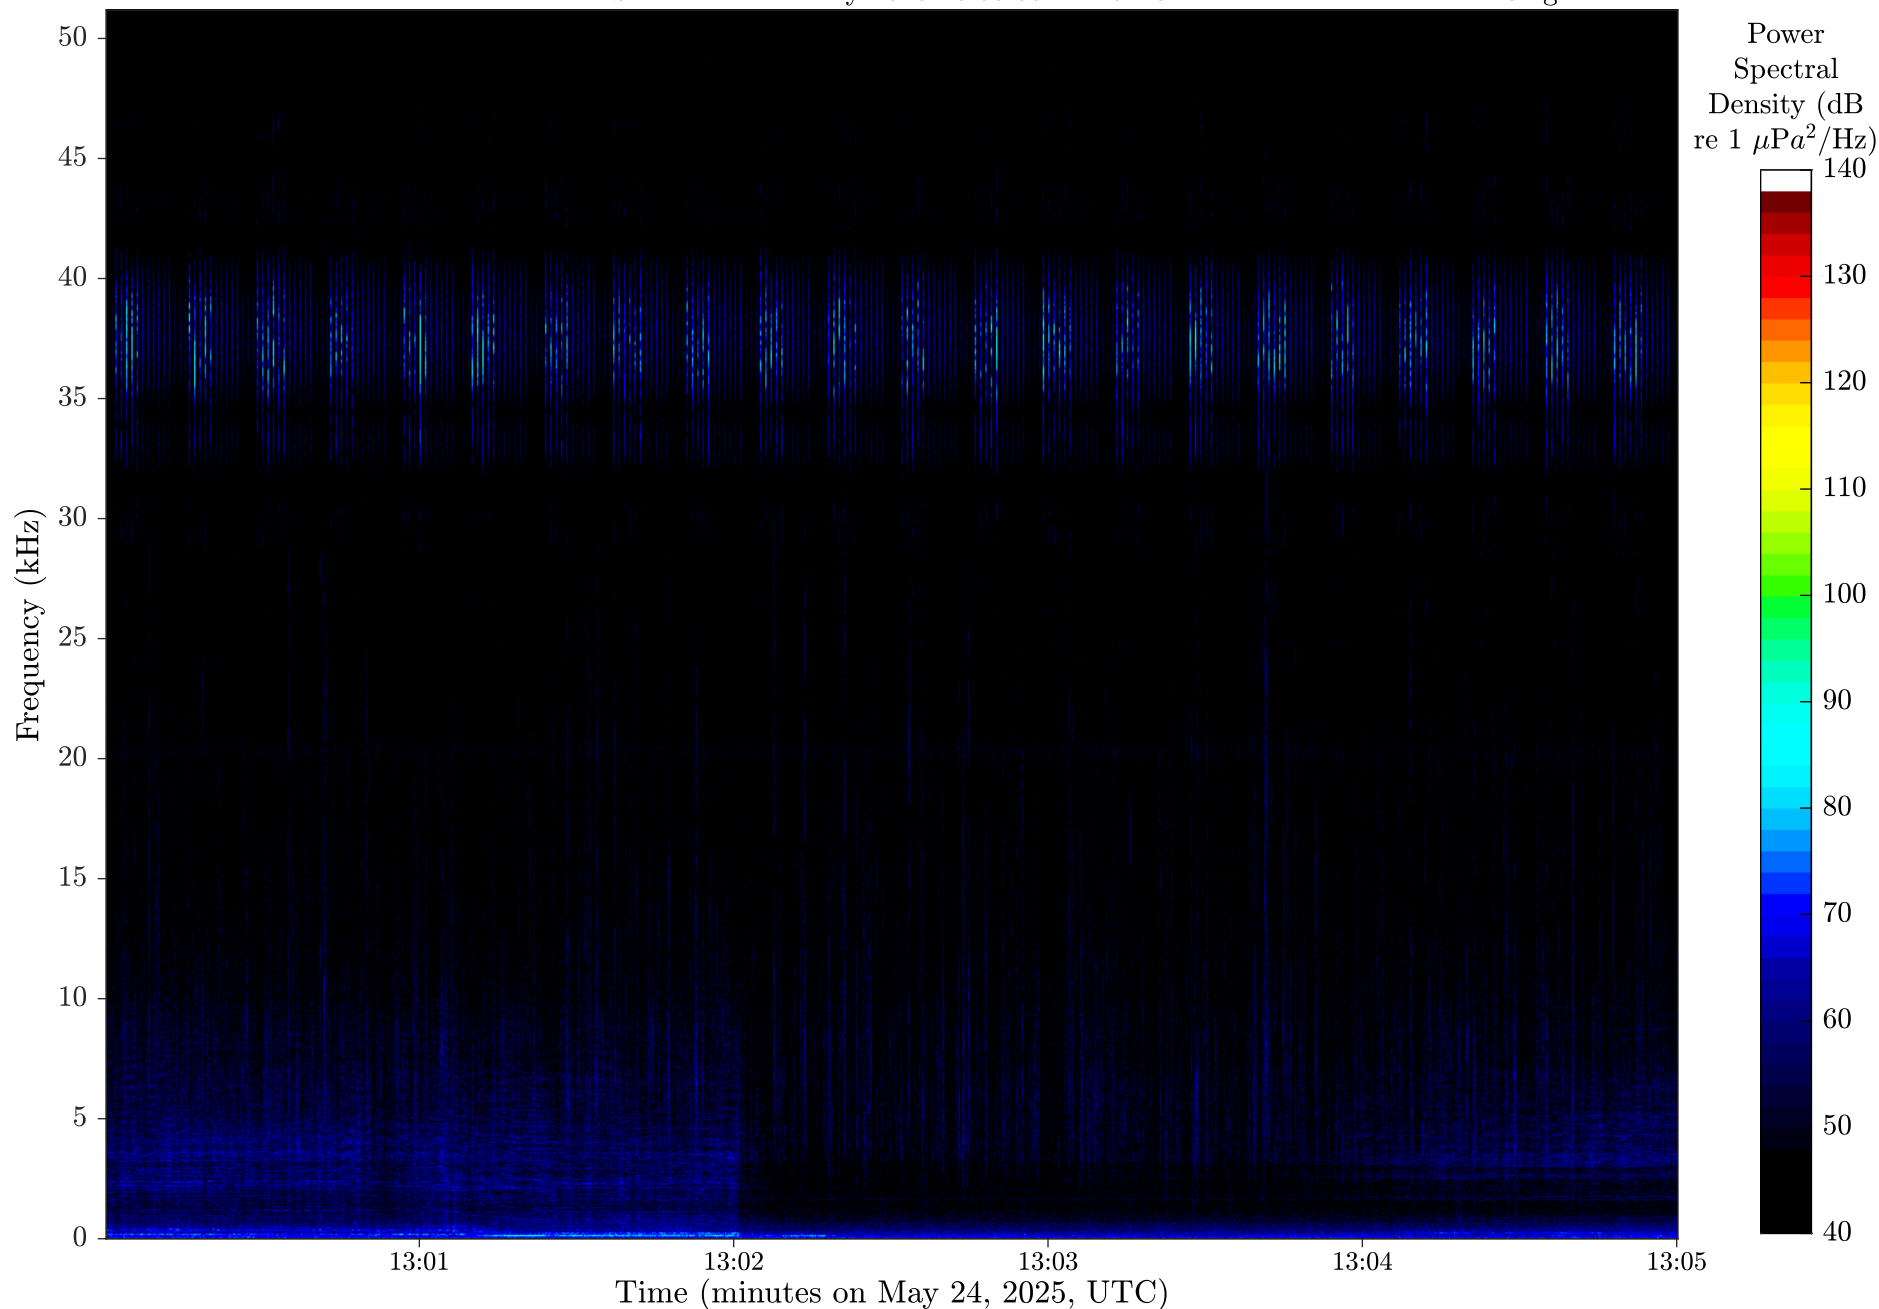


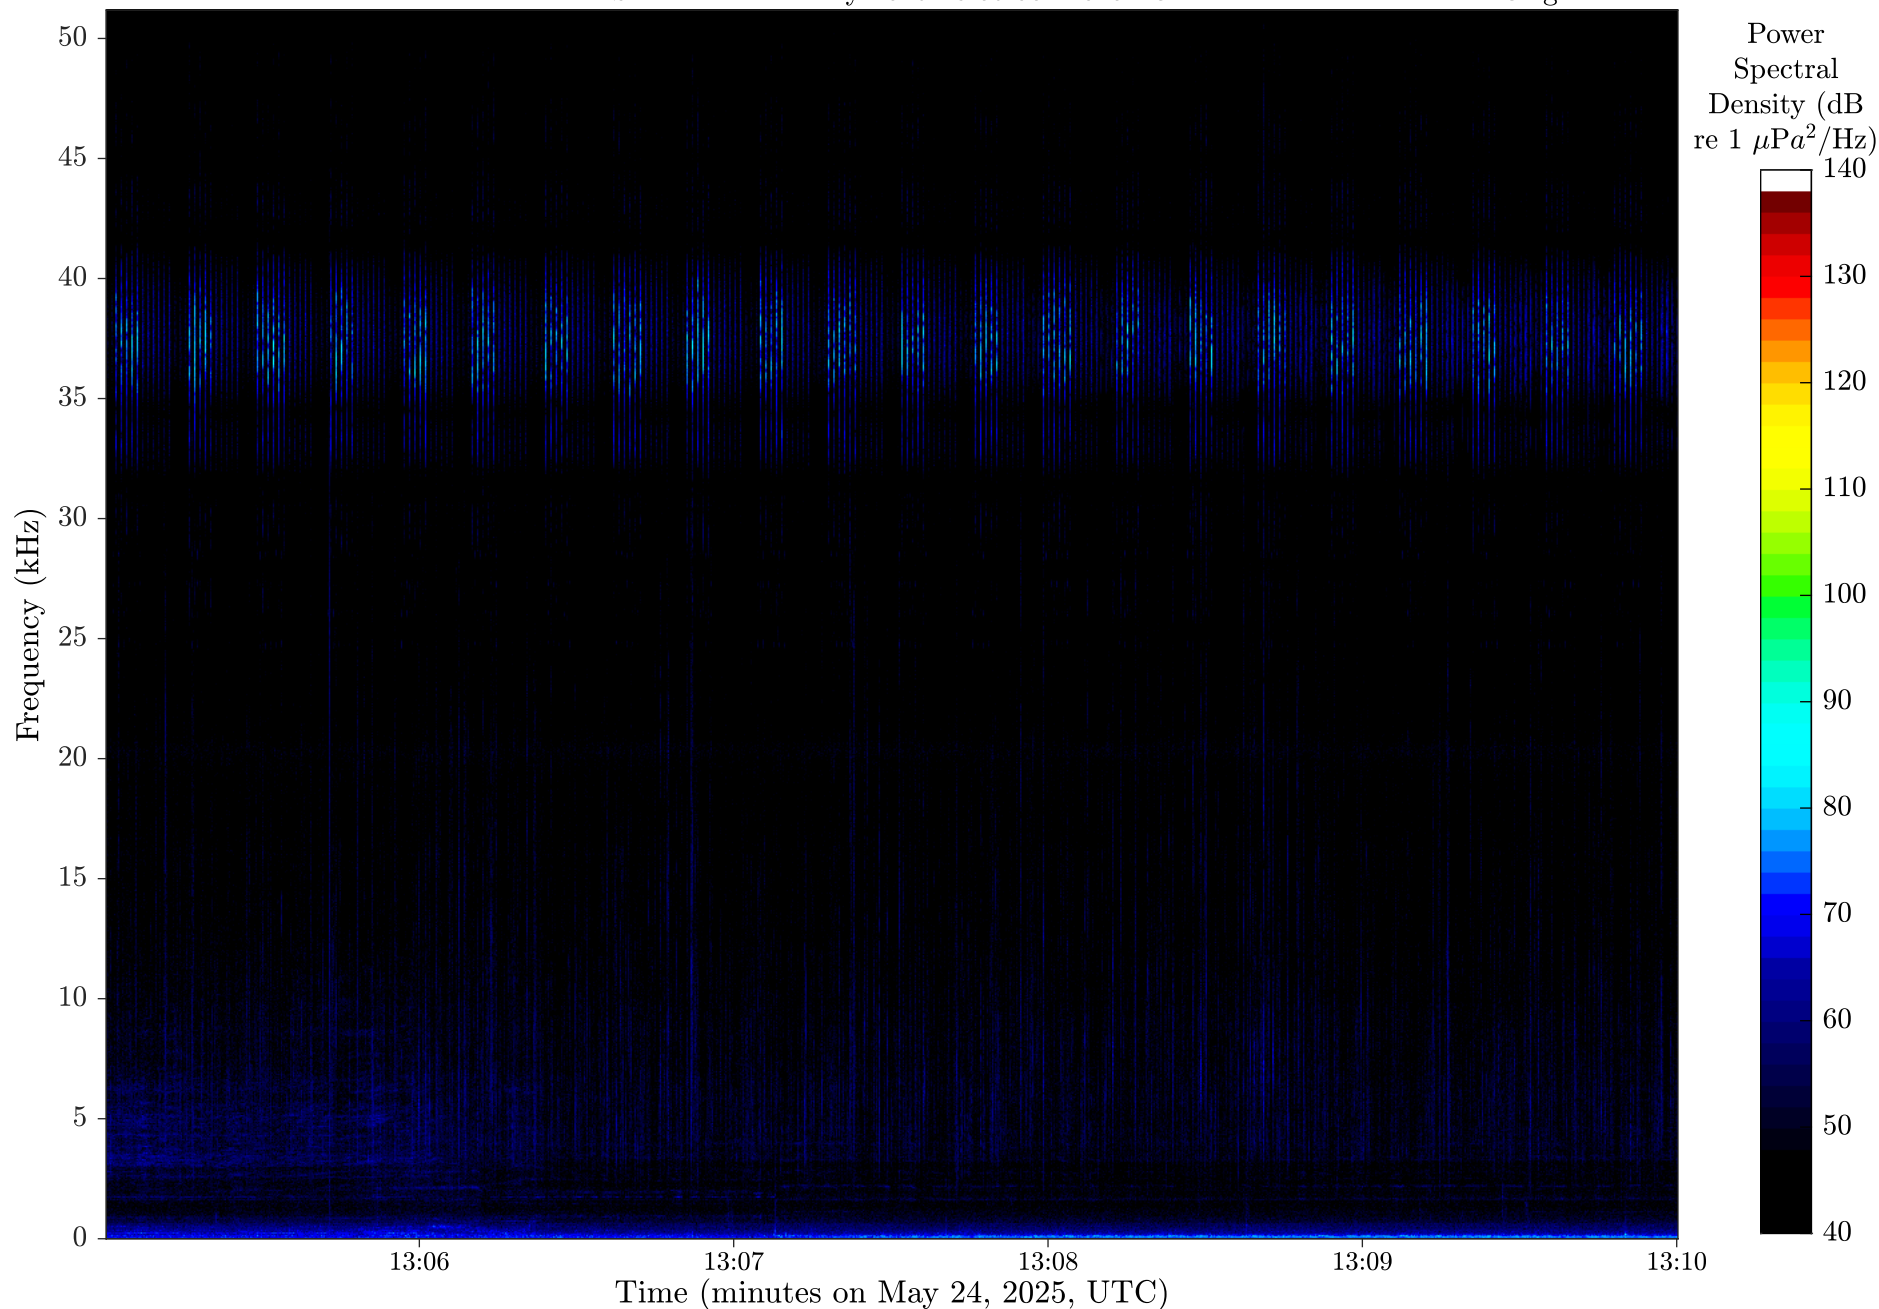

Comments: 31.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:31:23 UTC

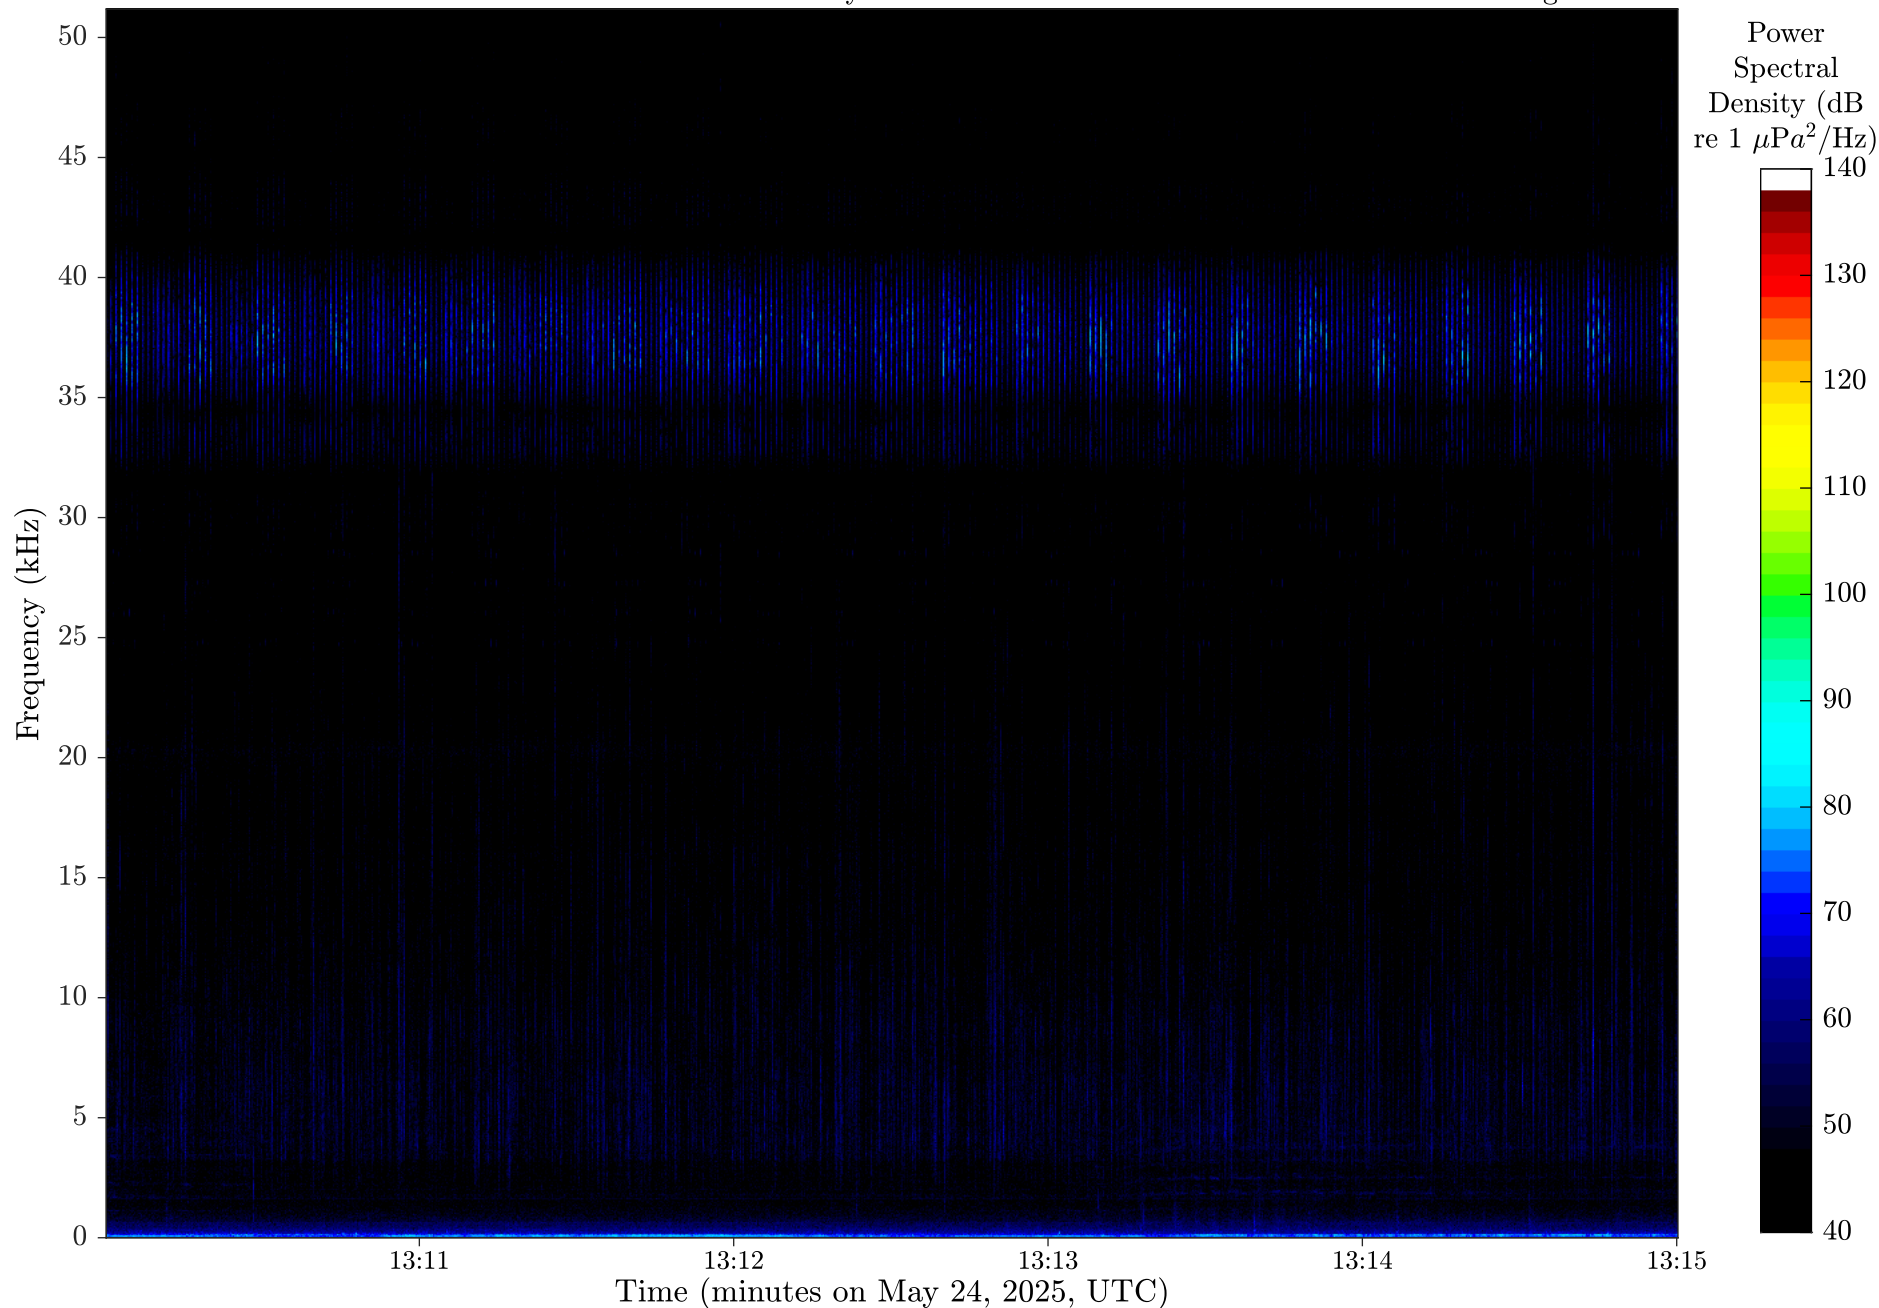

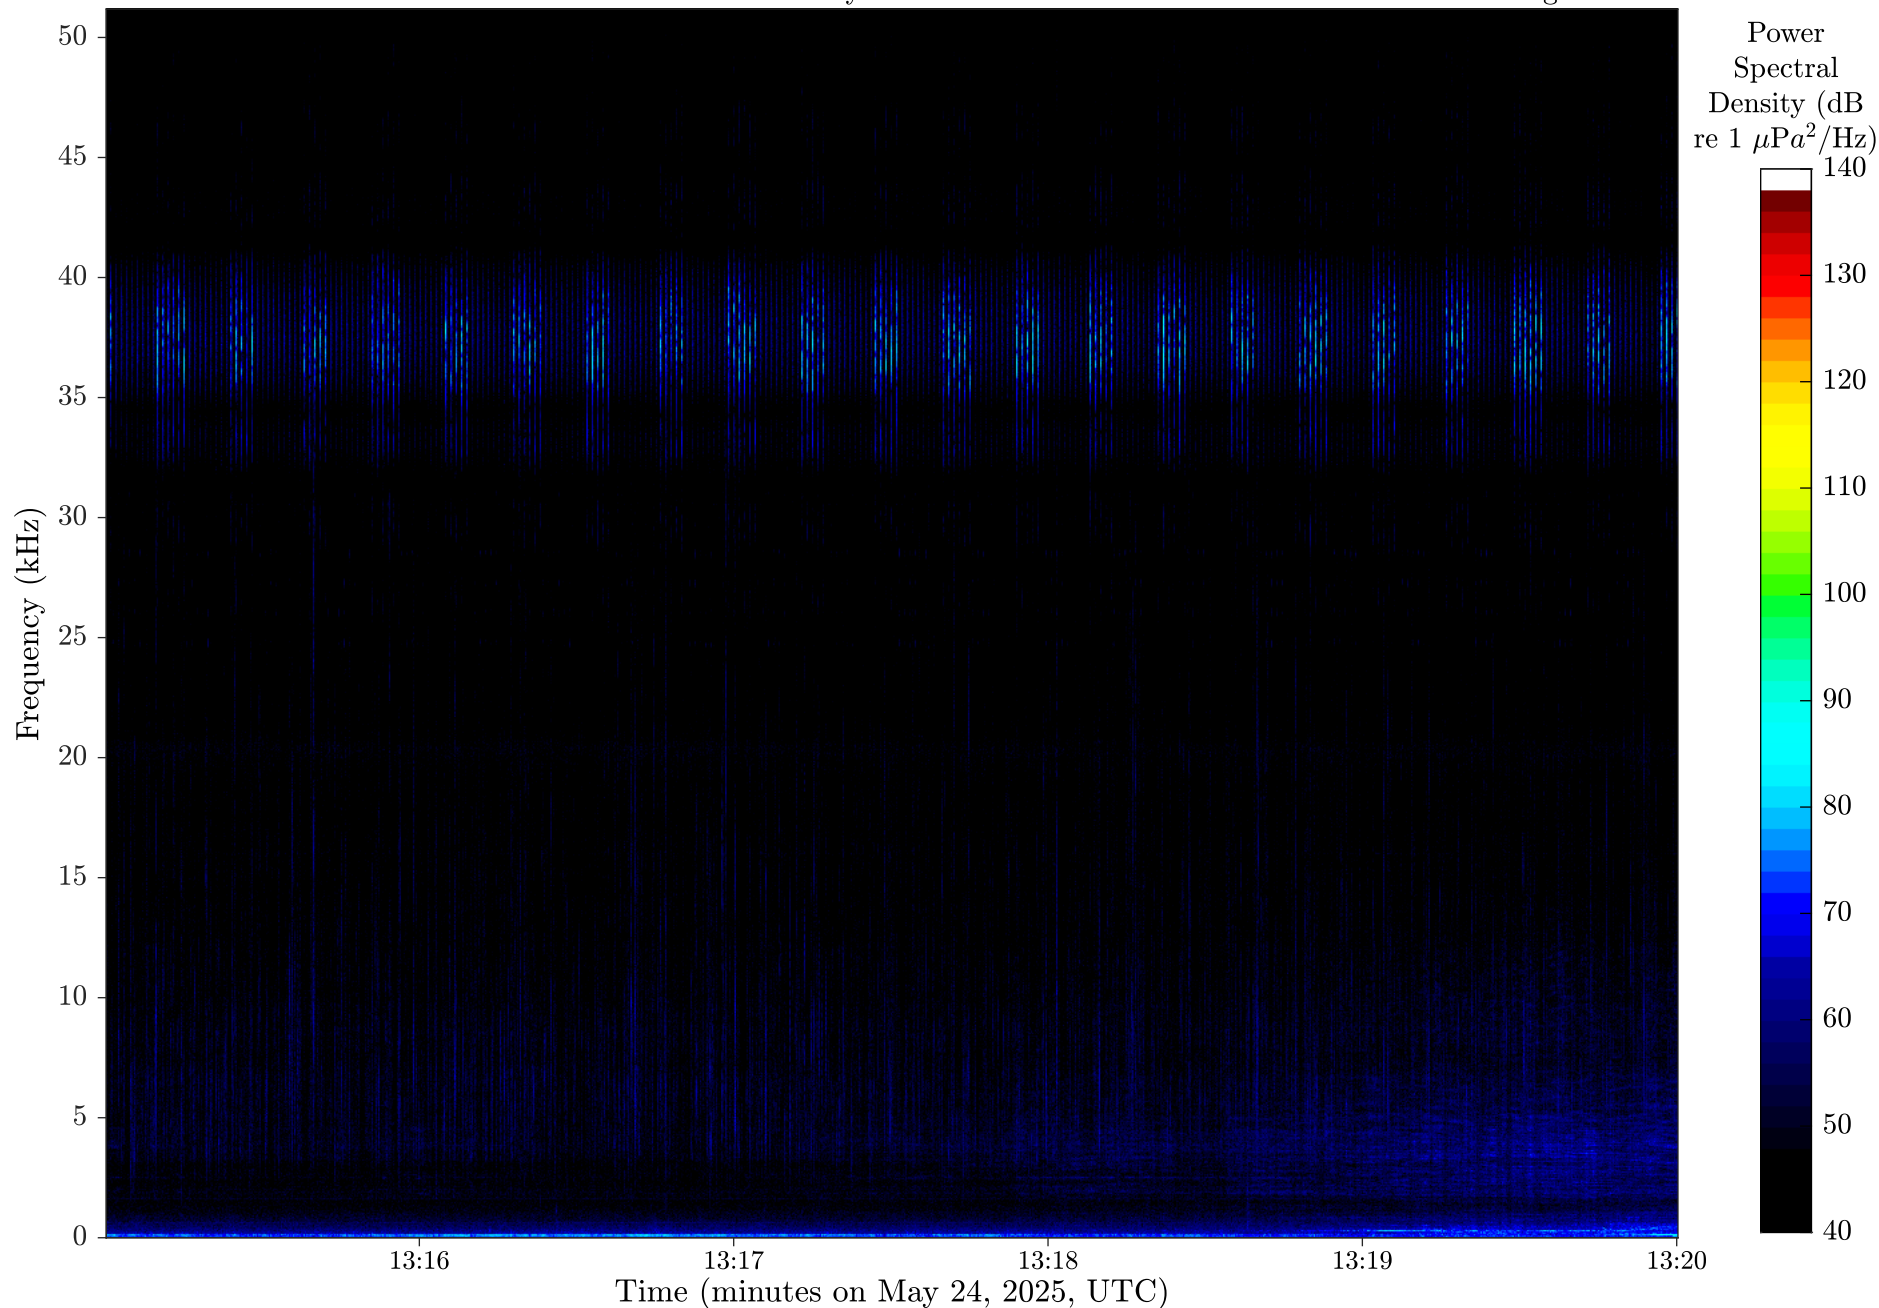


Comments: 30.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:37 UTC

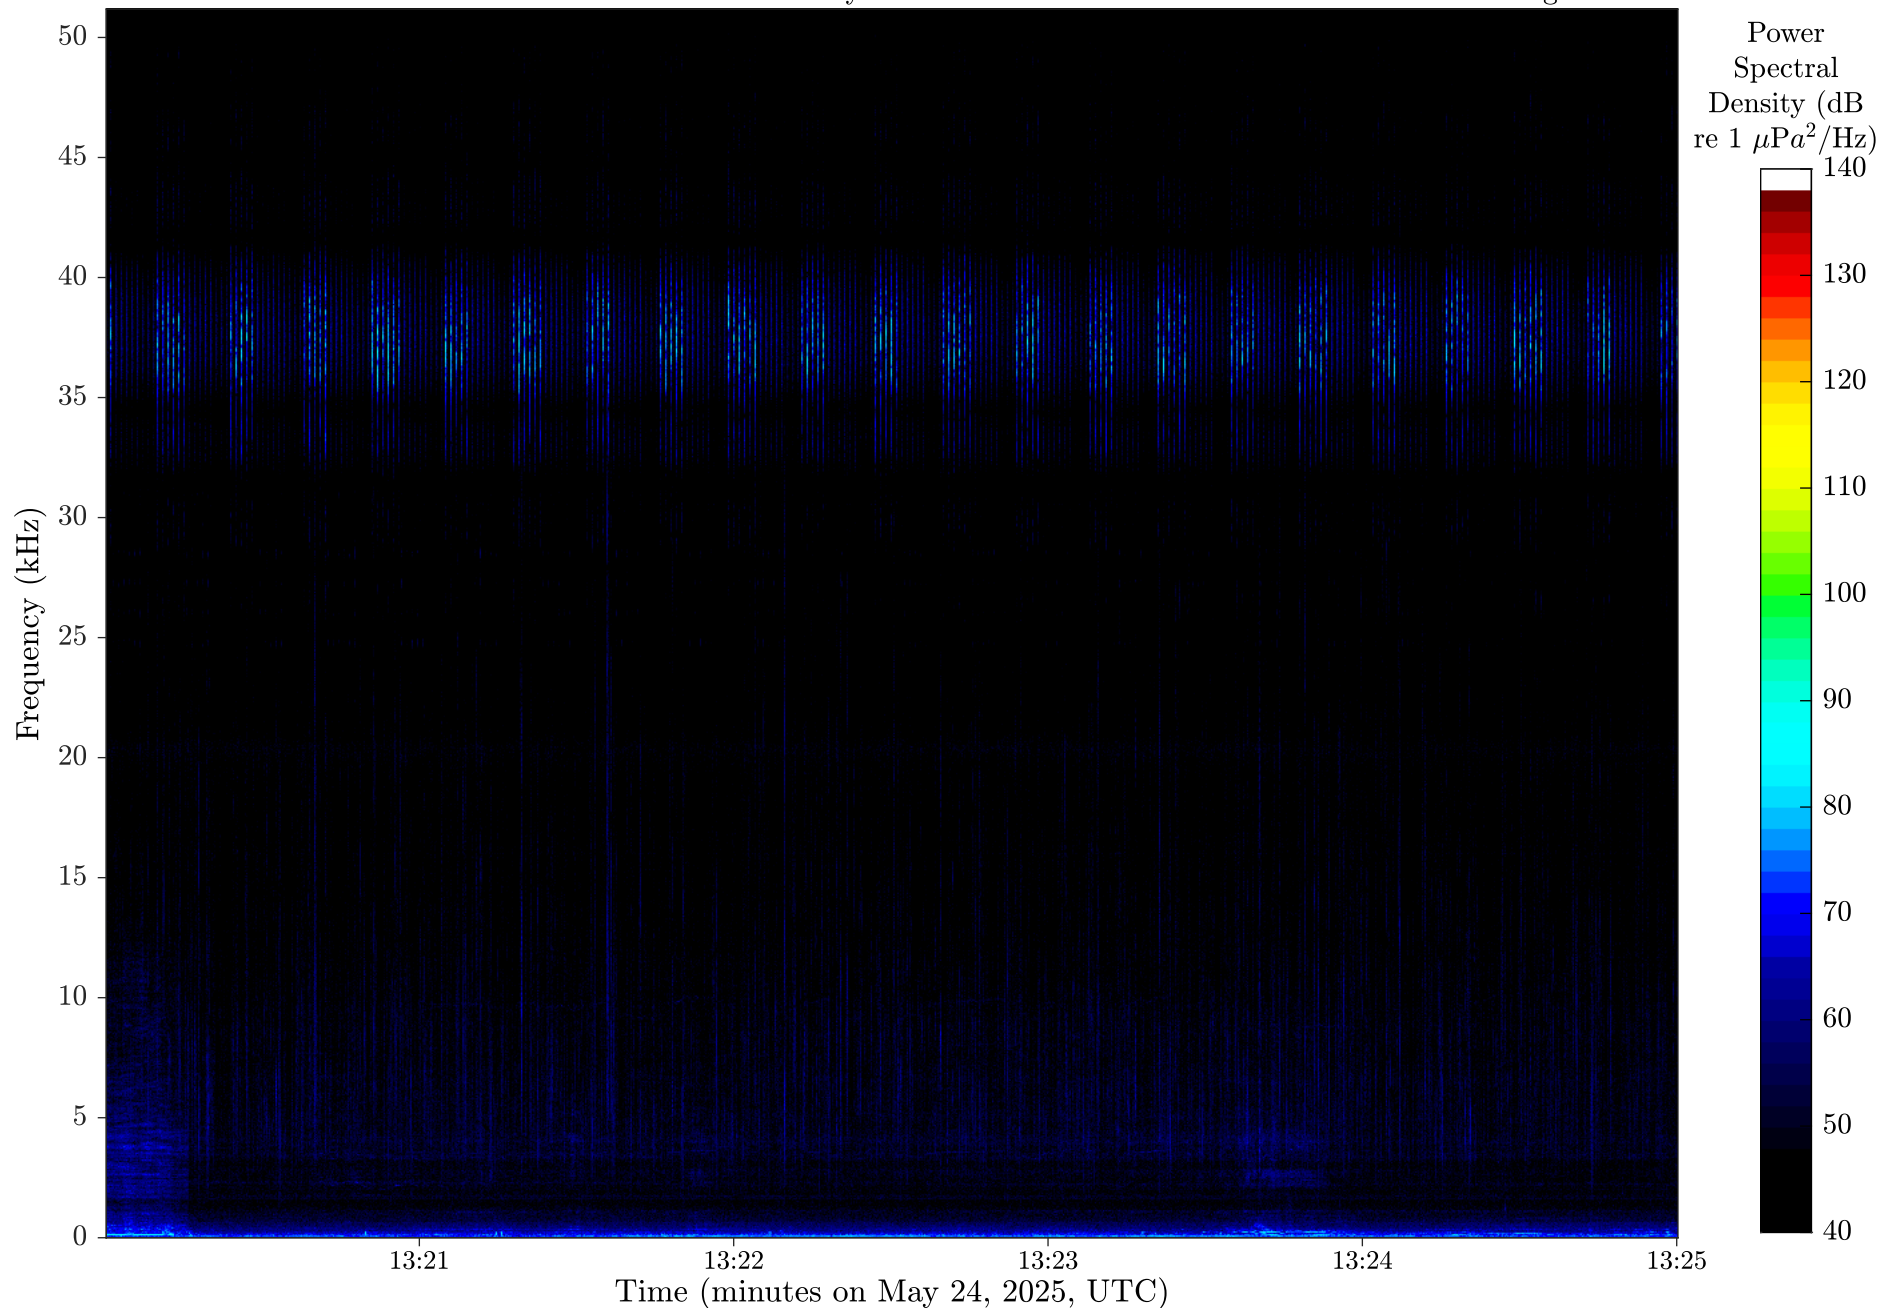


Comments: 31.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:45 UTC

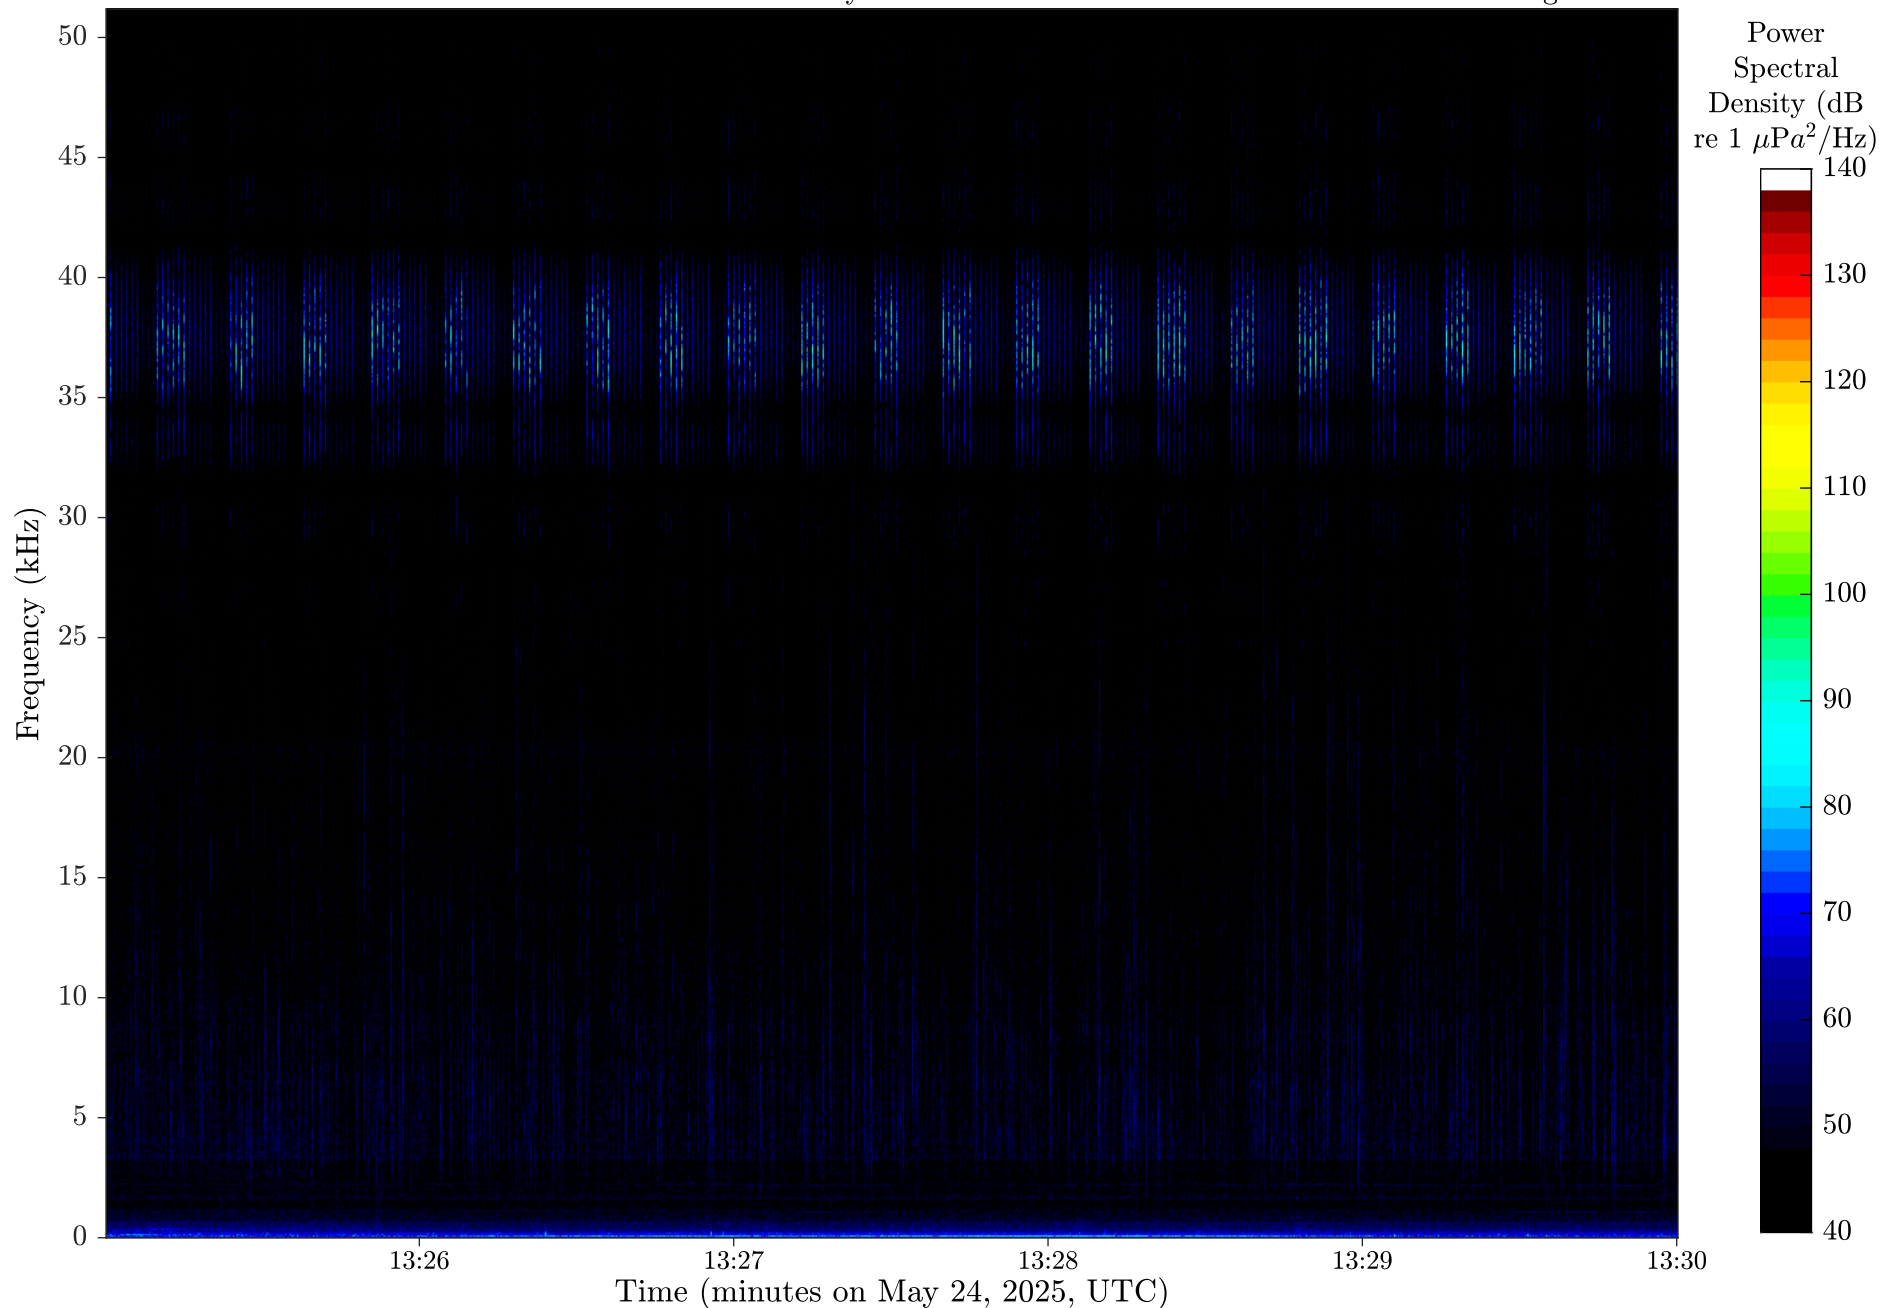


Comments: 32.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:31:52 UTC

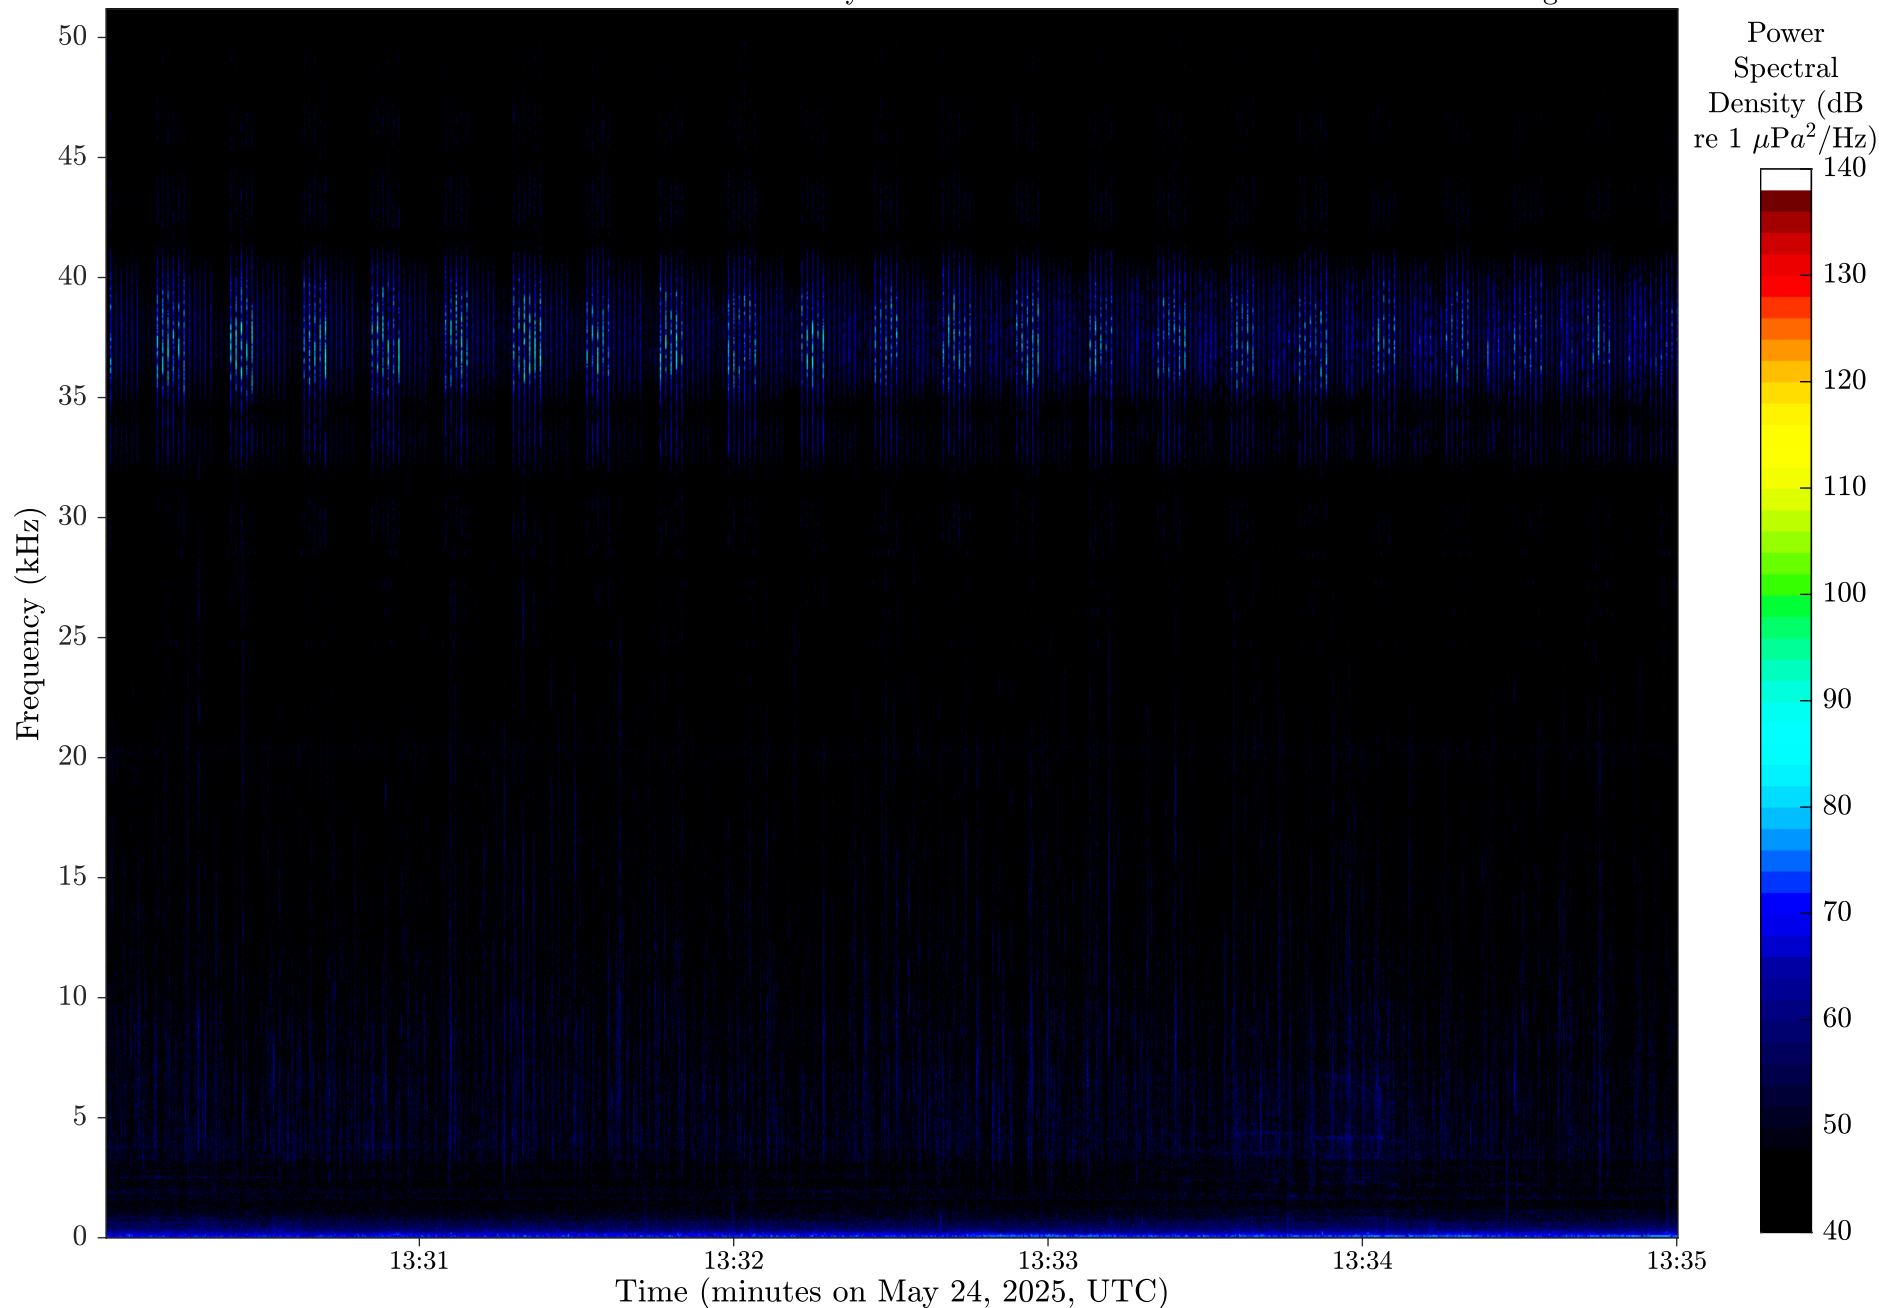

Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:32:00 UTC

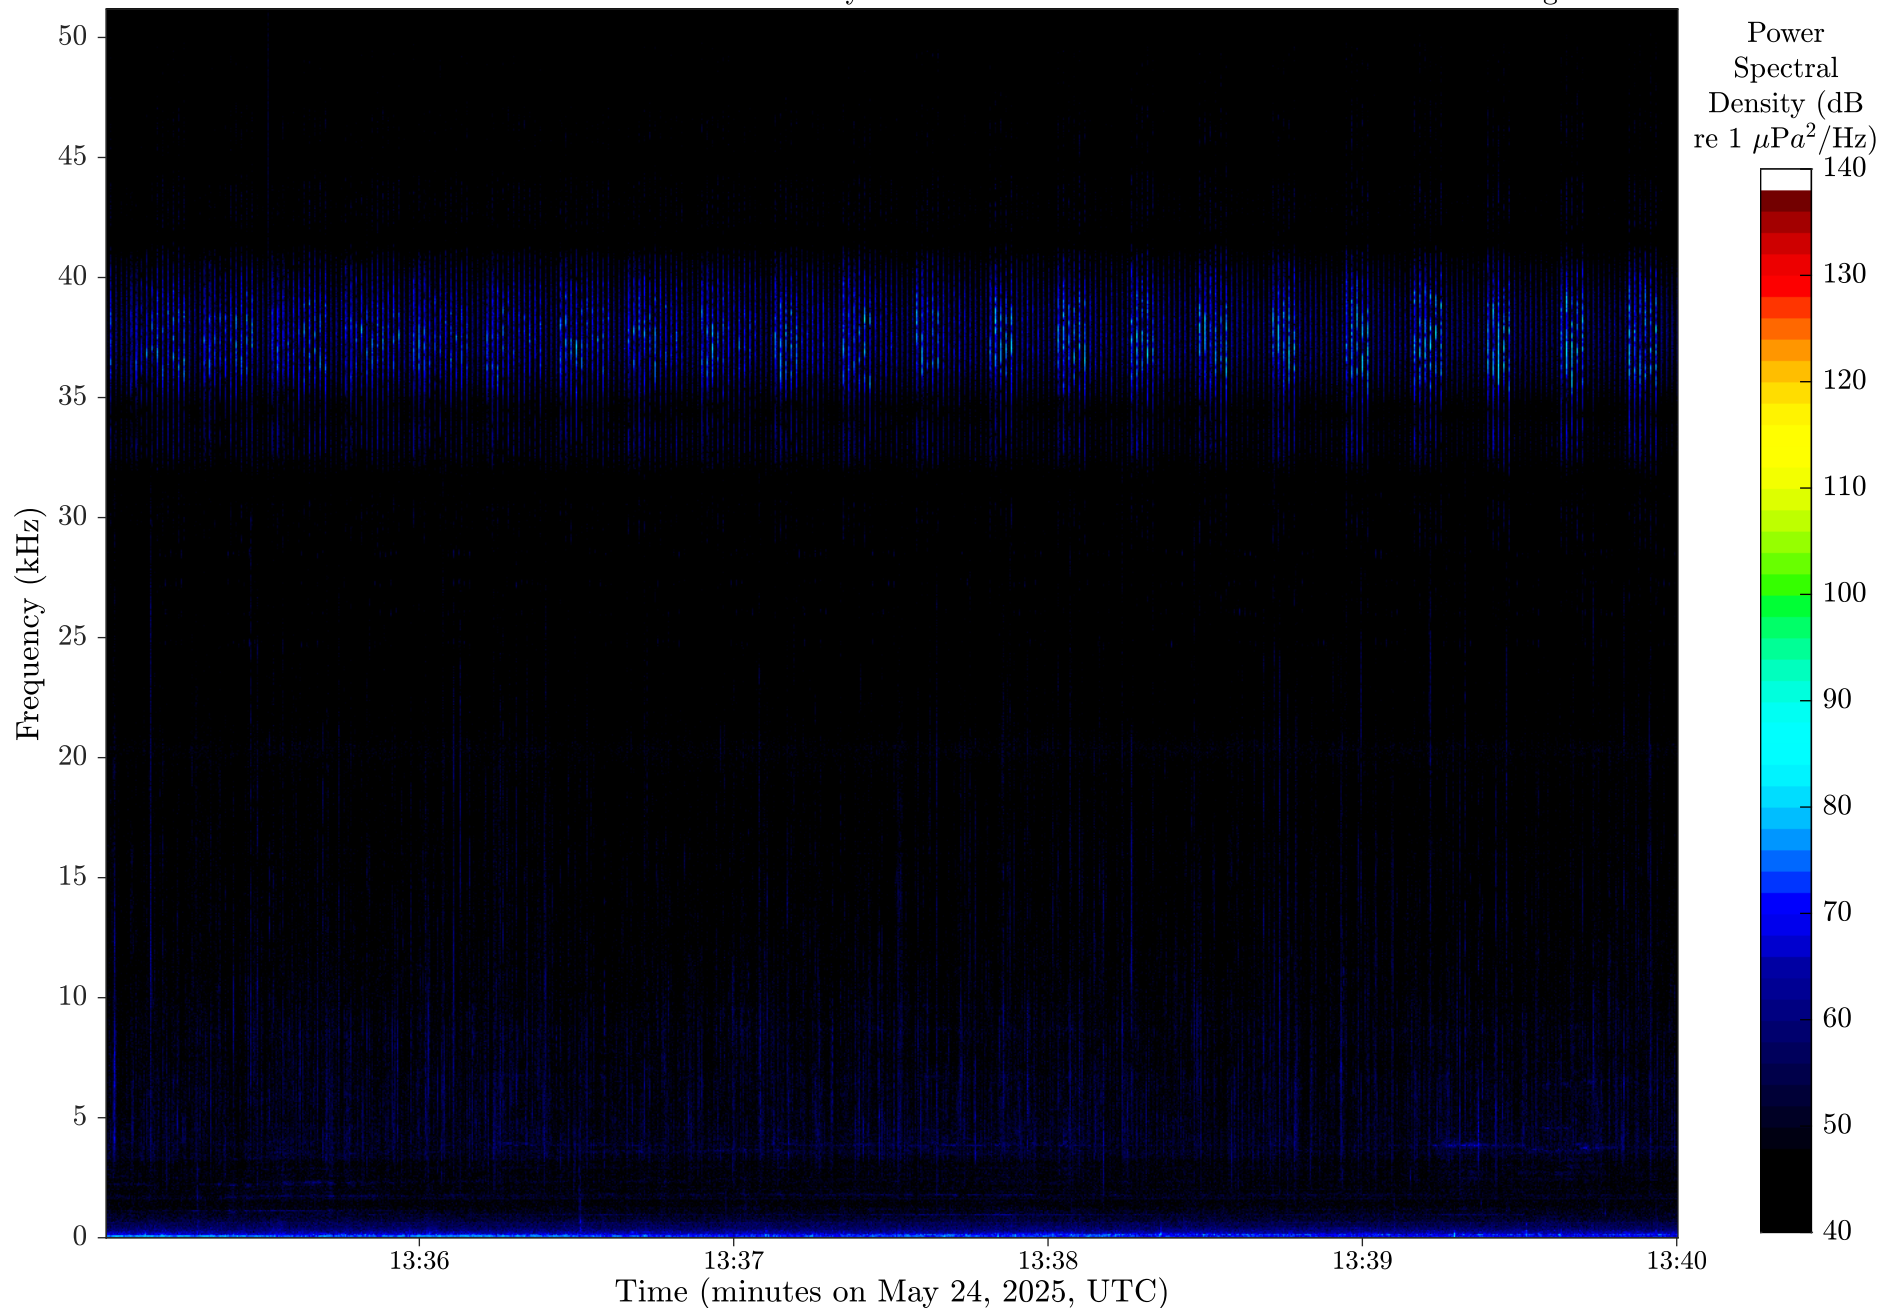


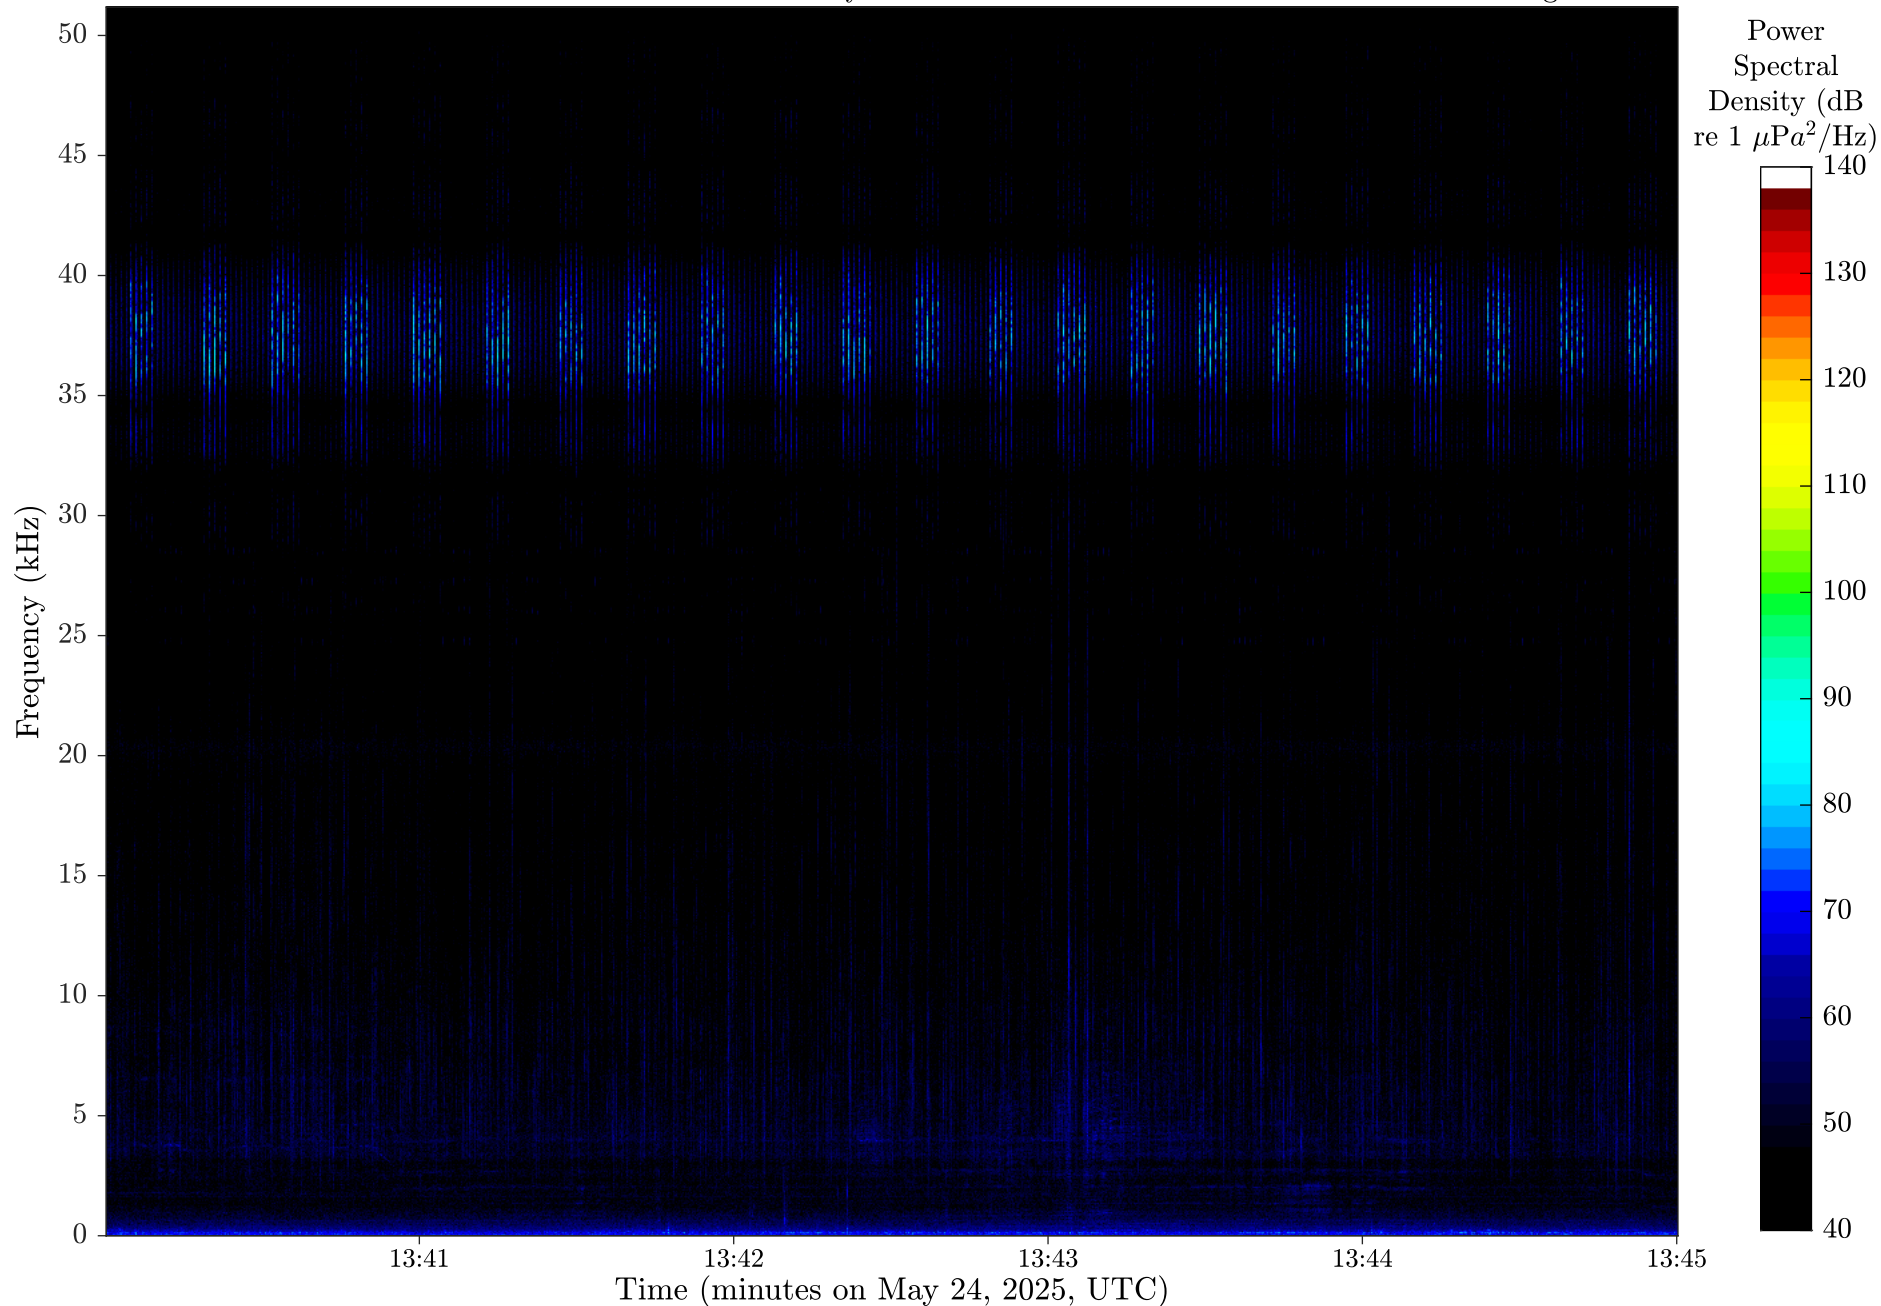

Comments: 31.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:32:14 UTC

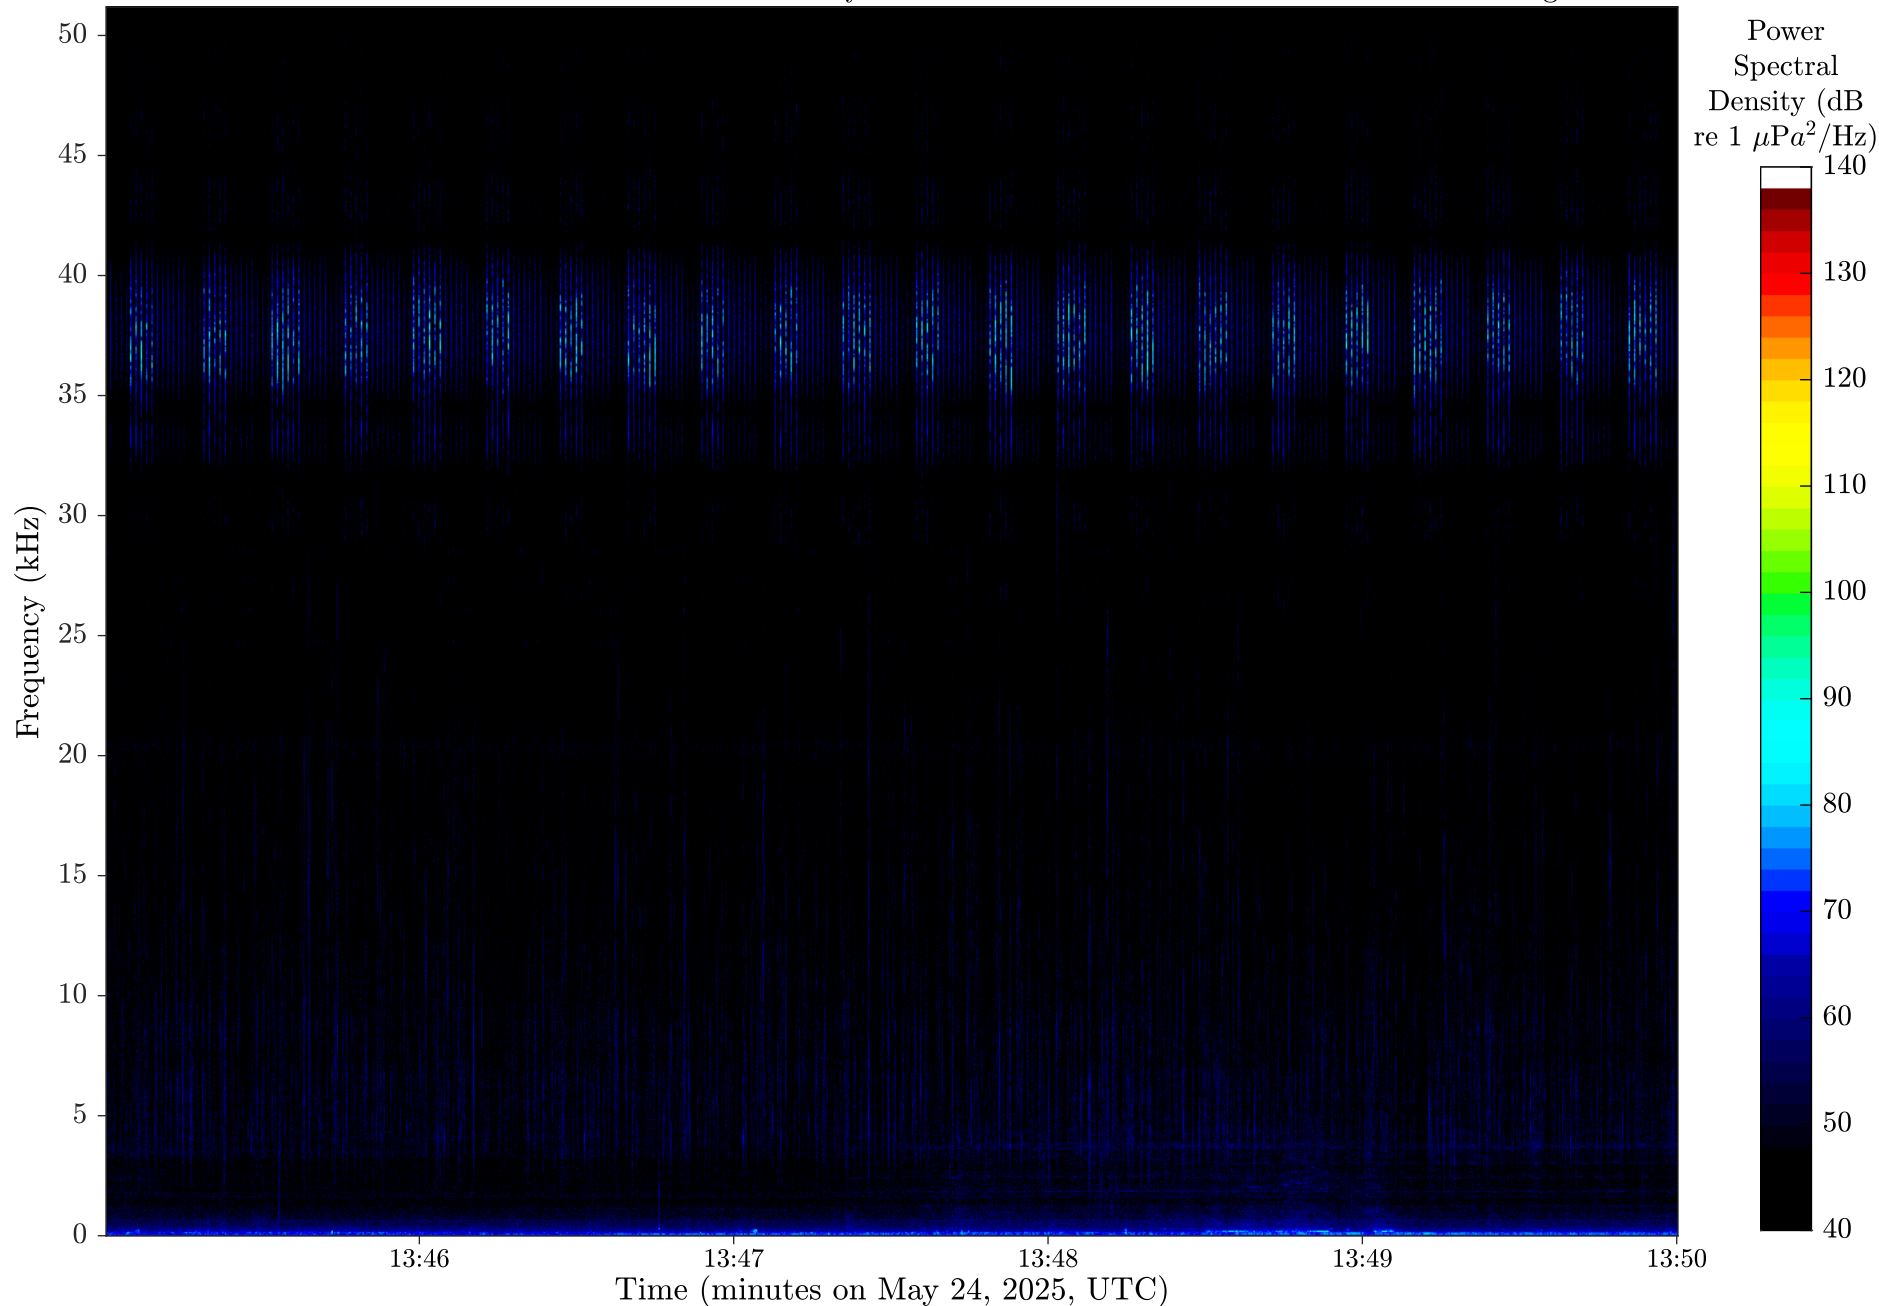

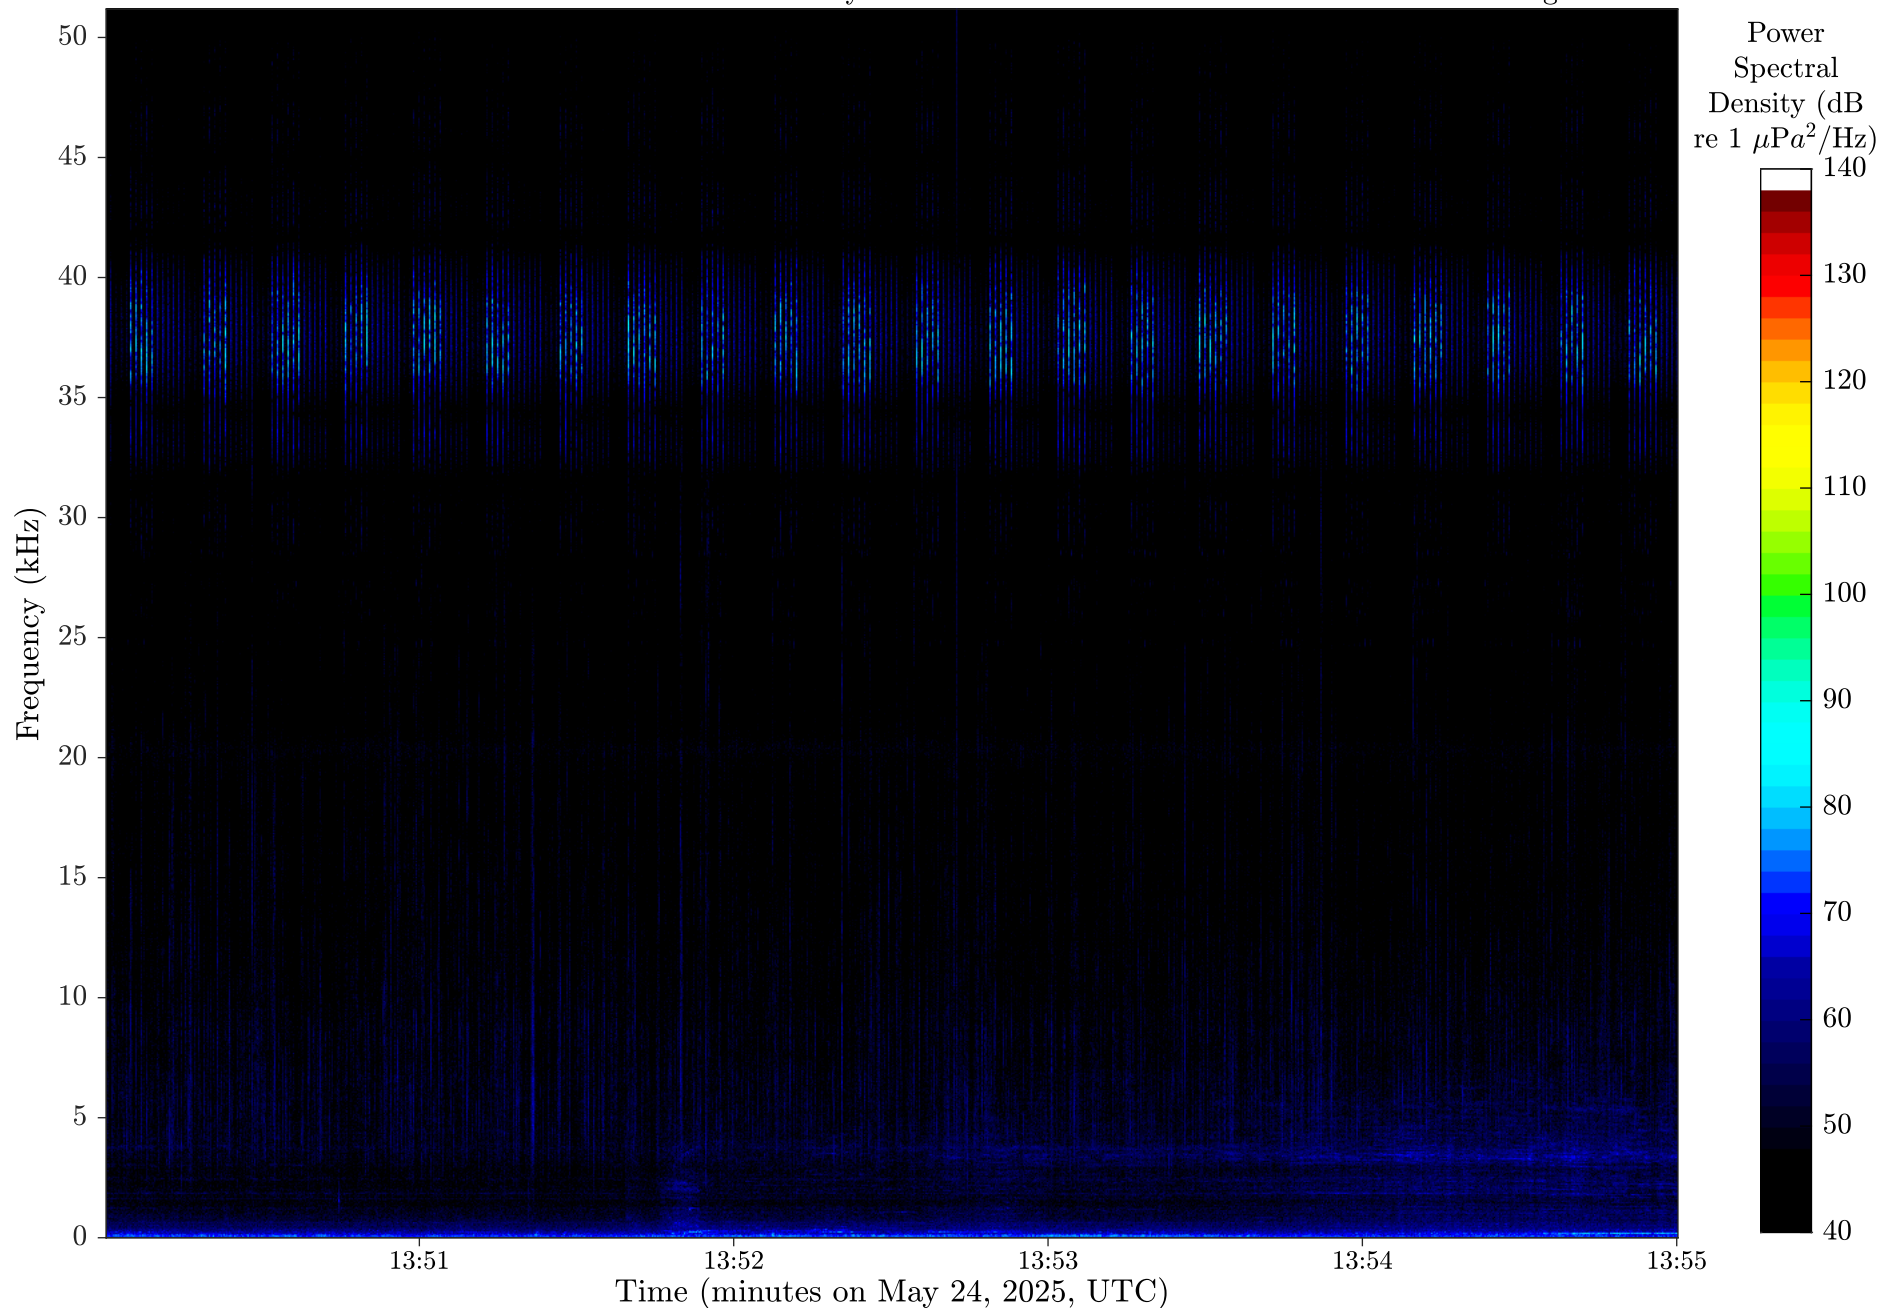


Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:32:28 UTC

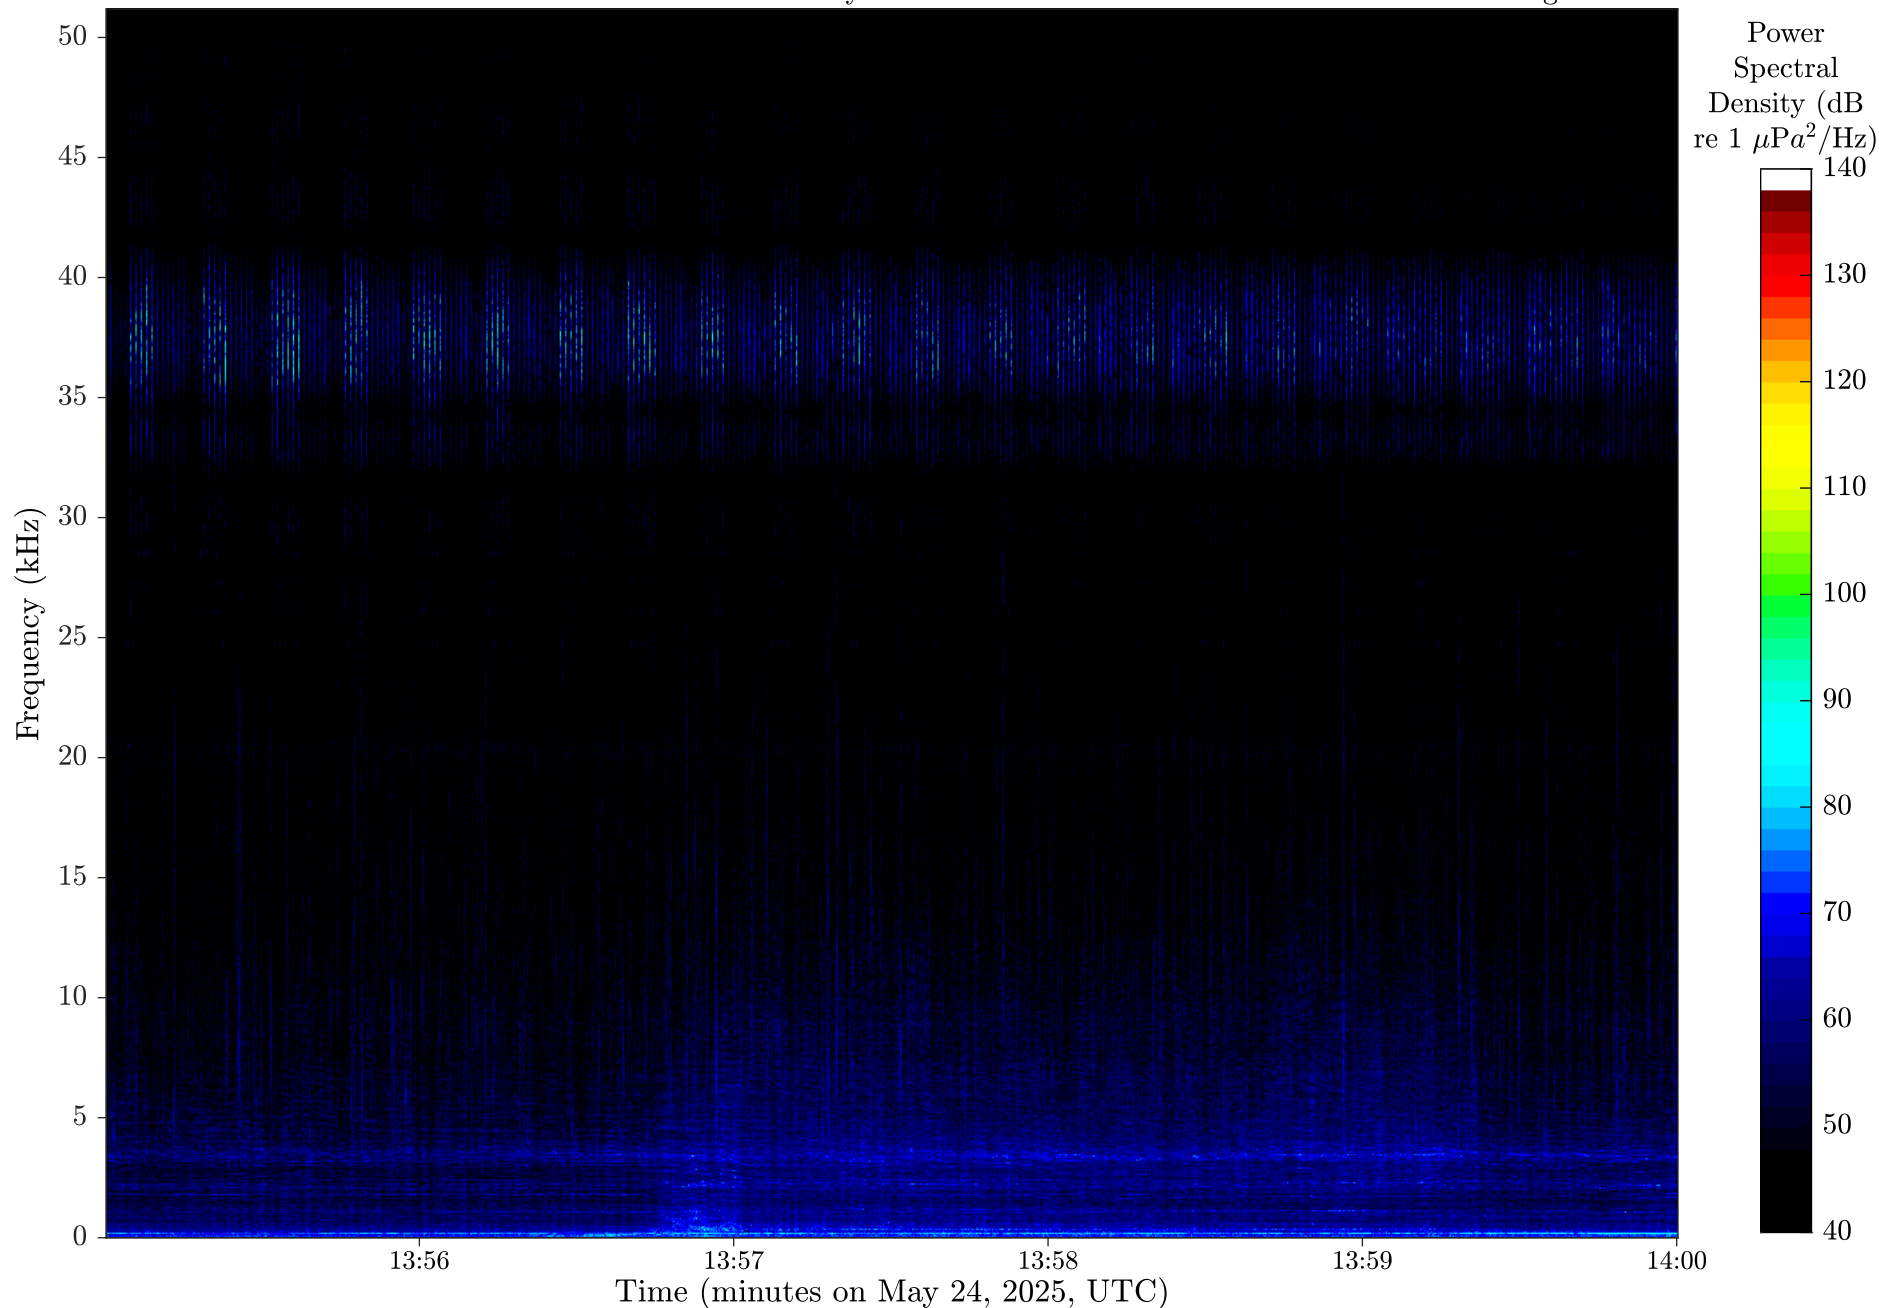


Comments: 29.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:32:36 UTC

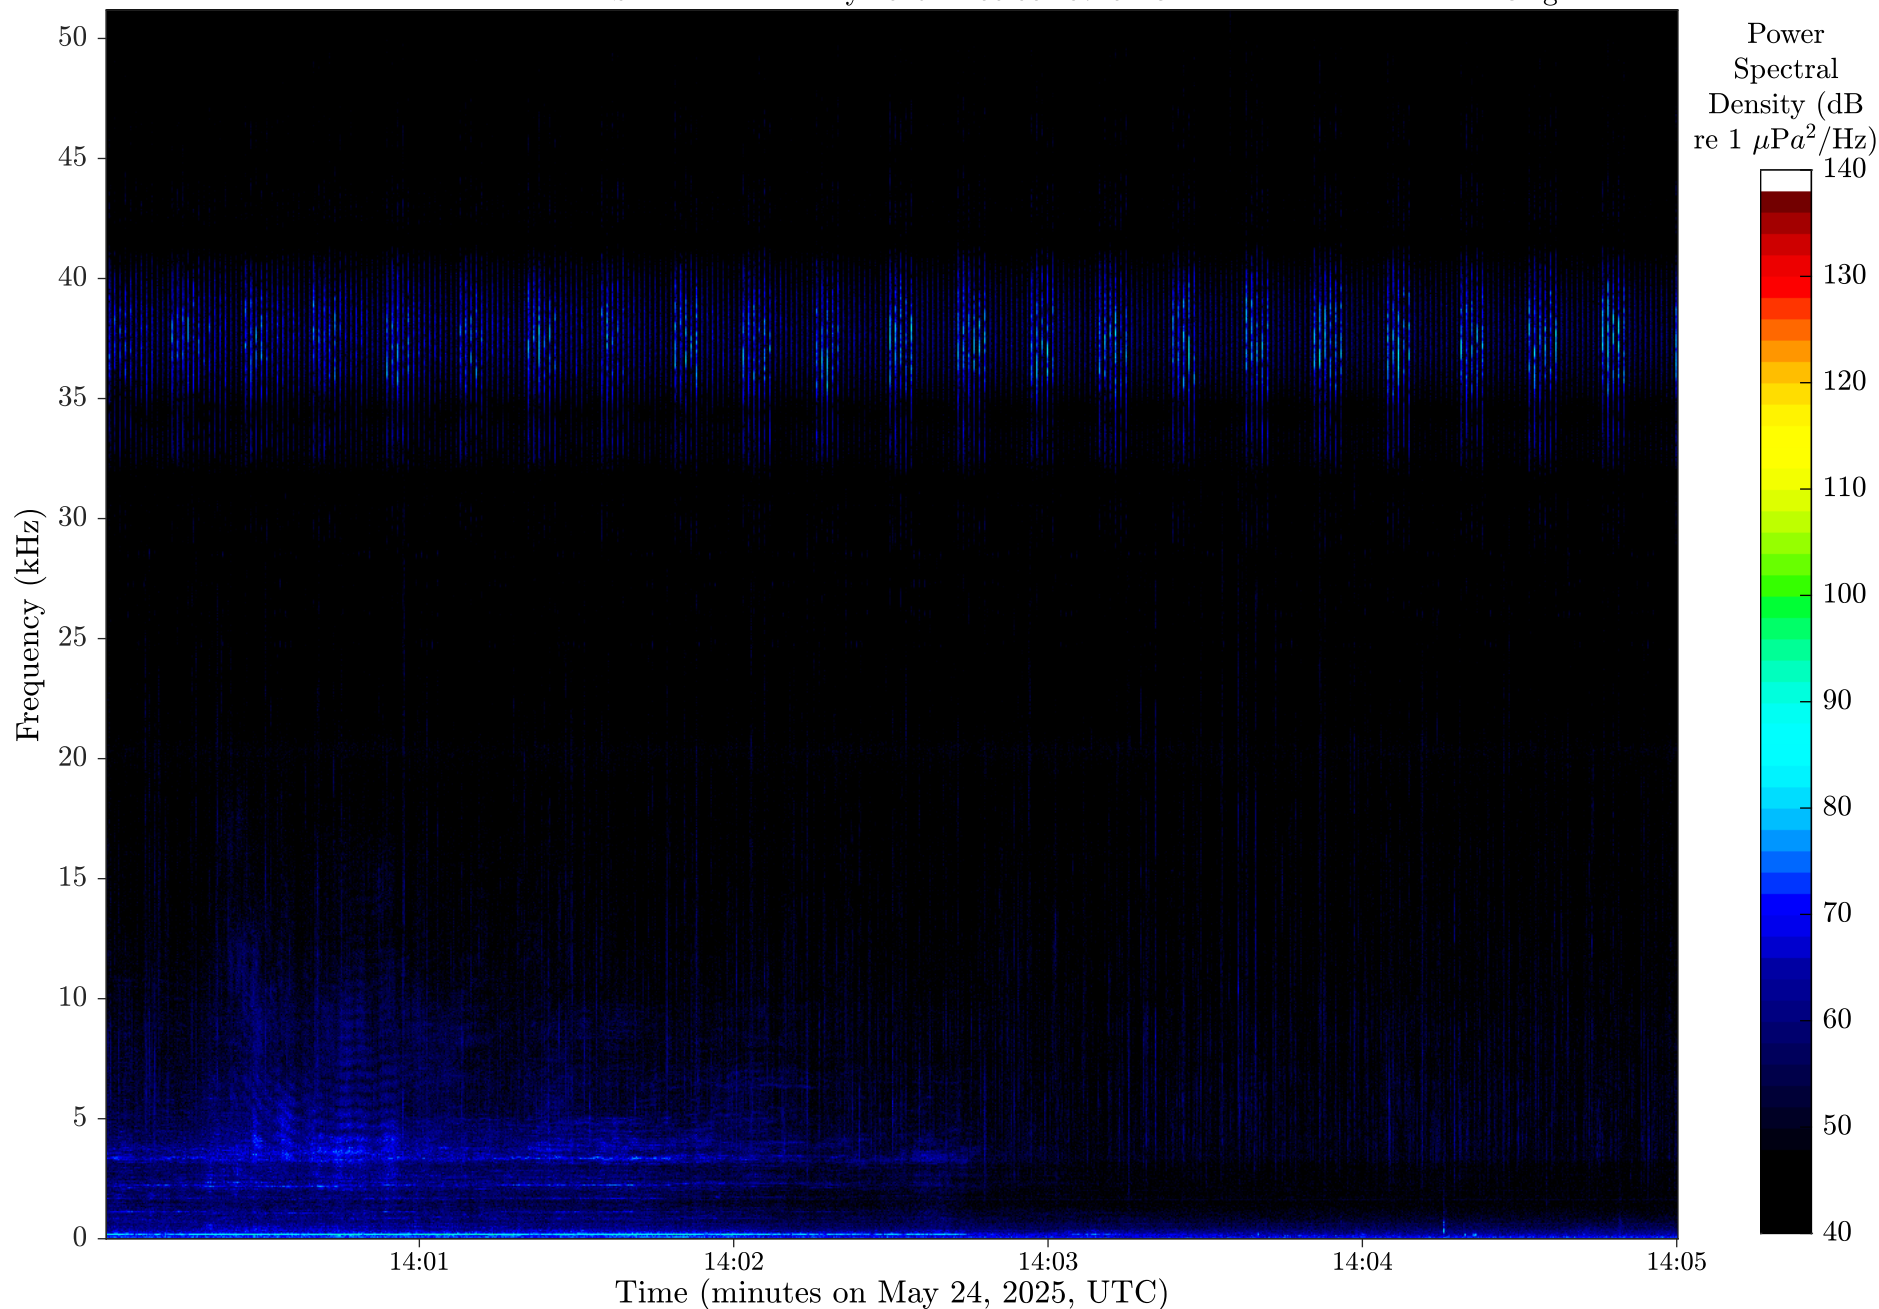


Comments: 31.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:32:43 UTC

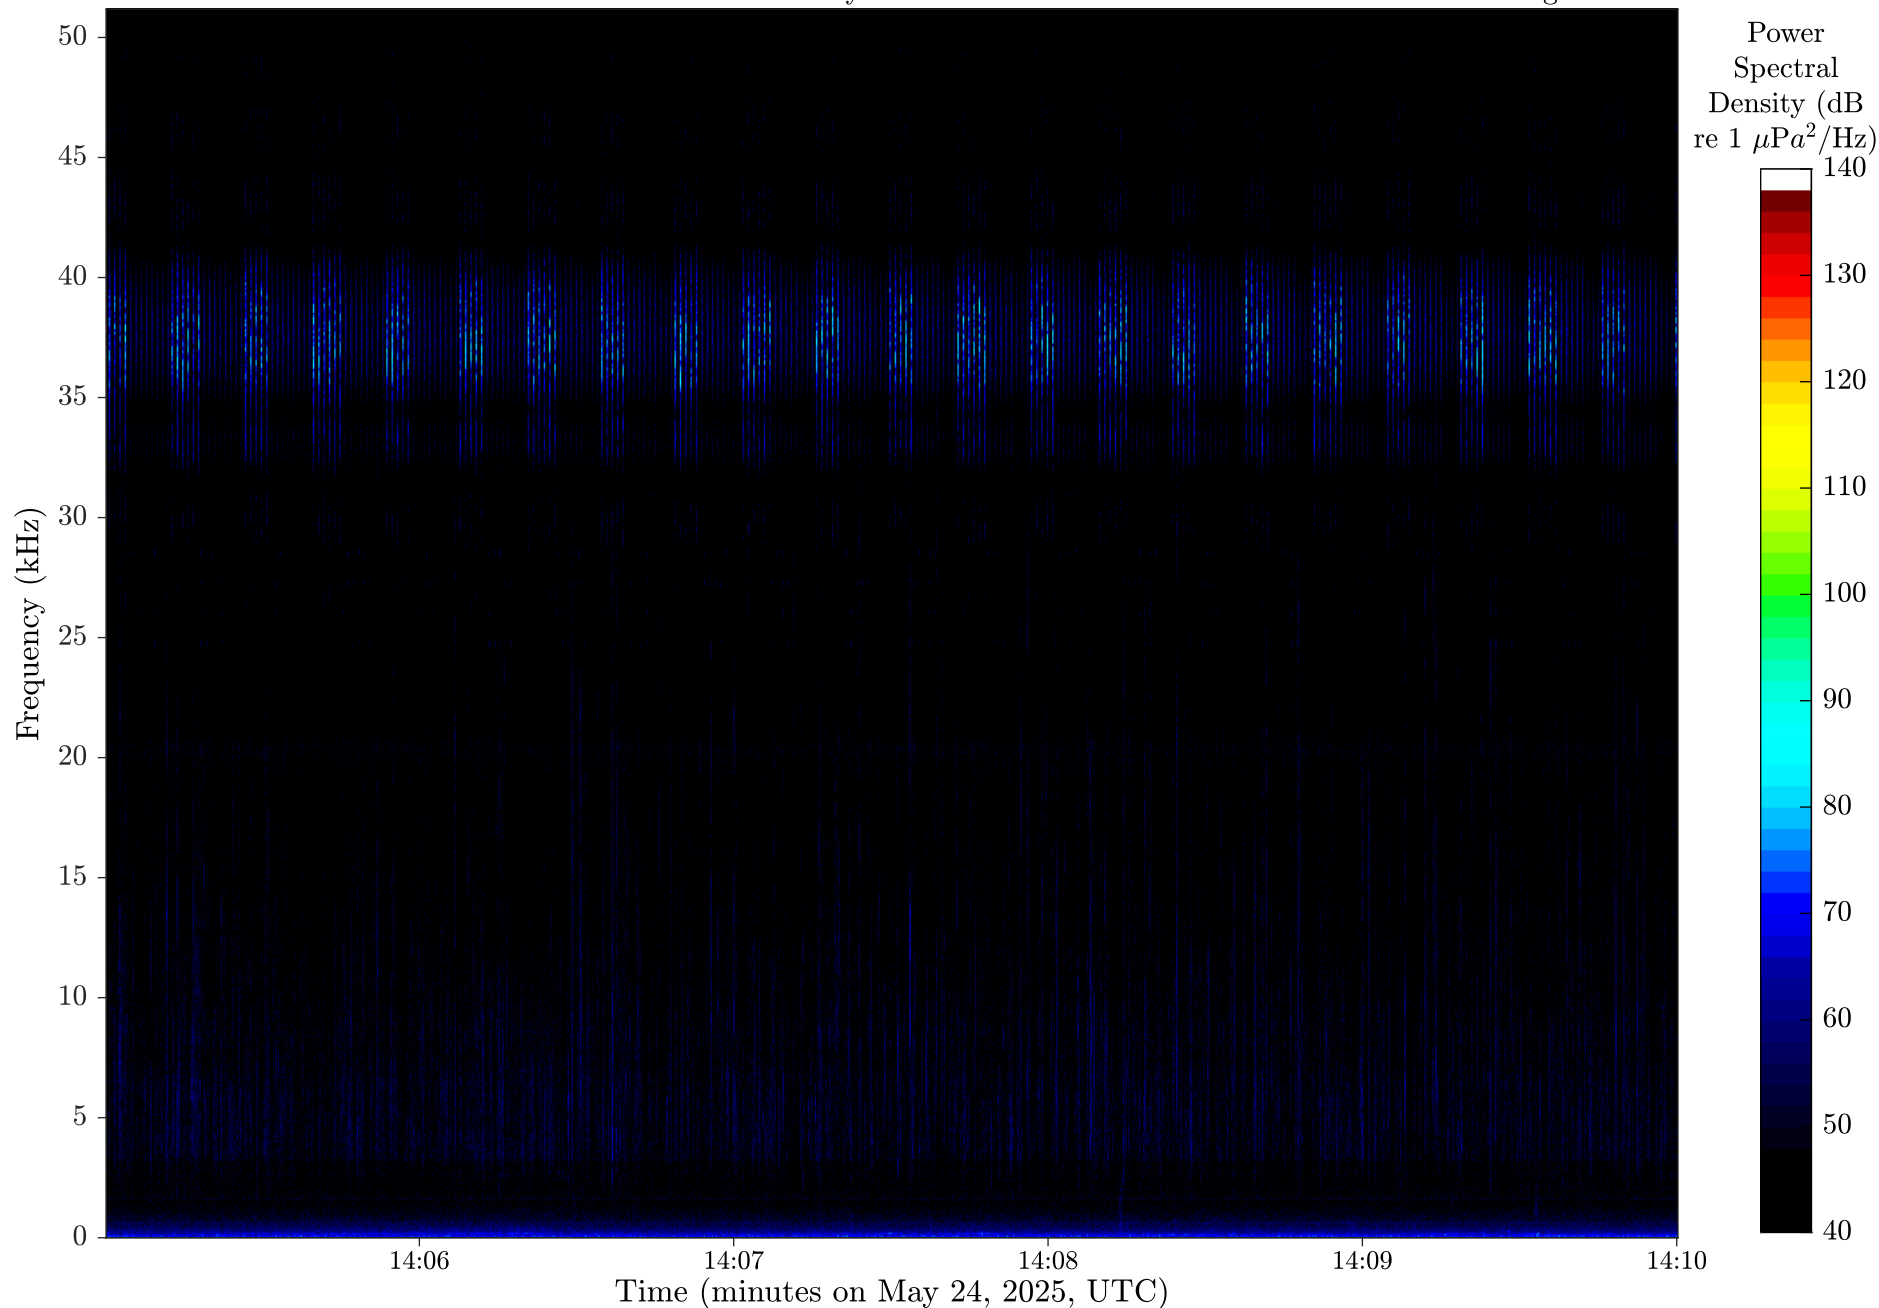

Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:32:50 UTC

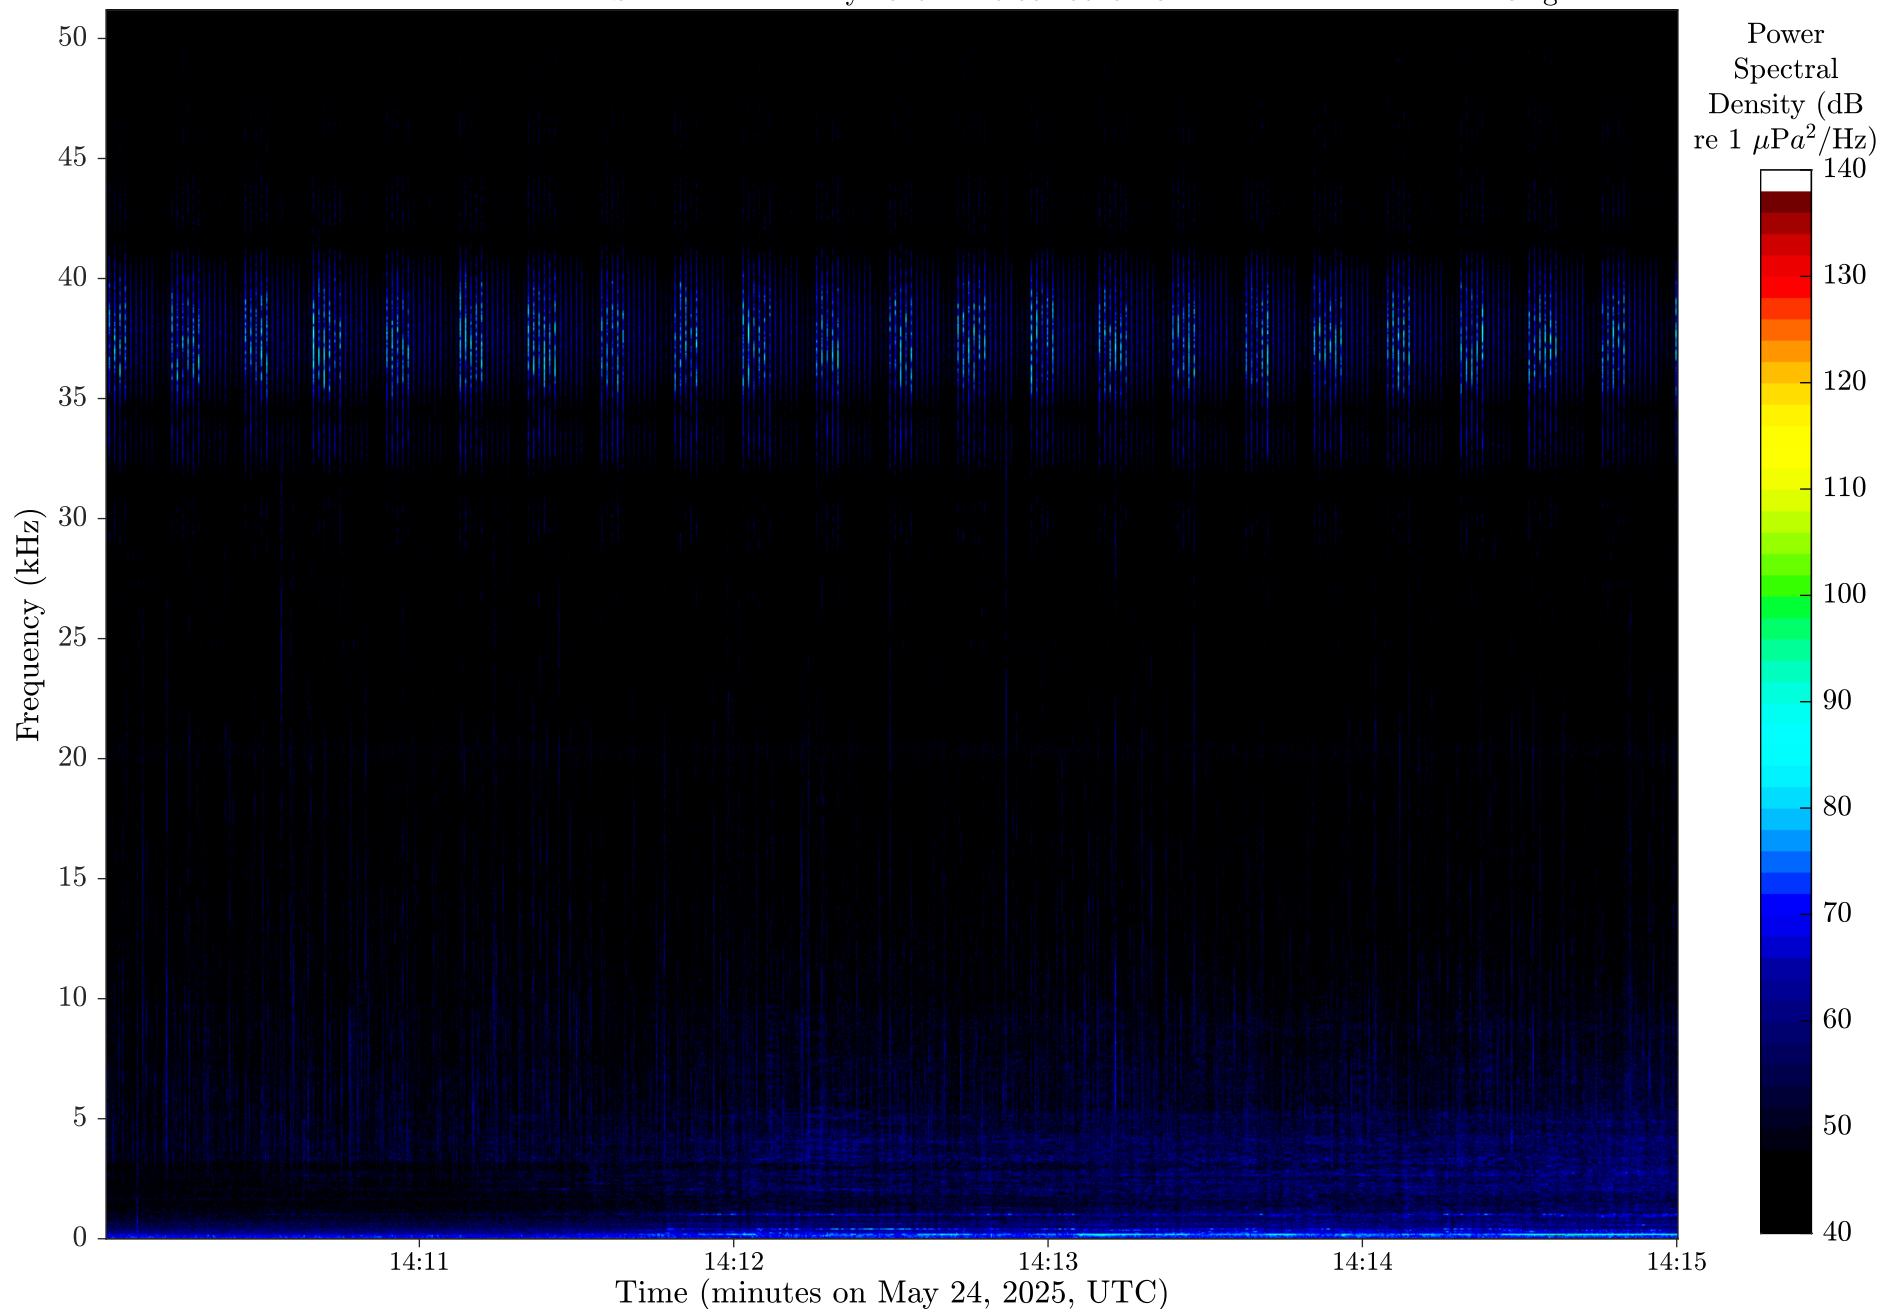

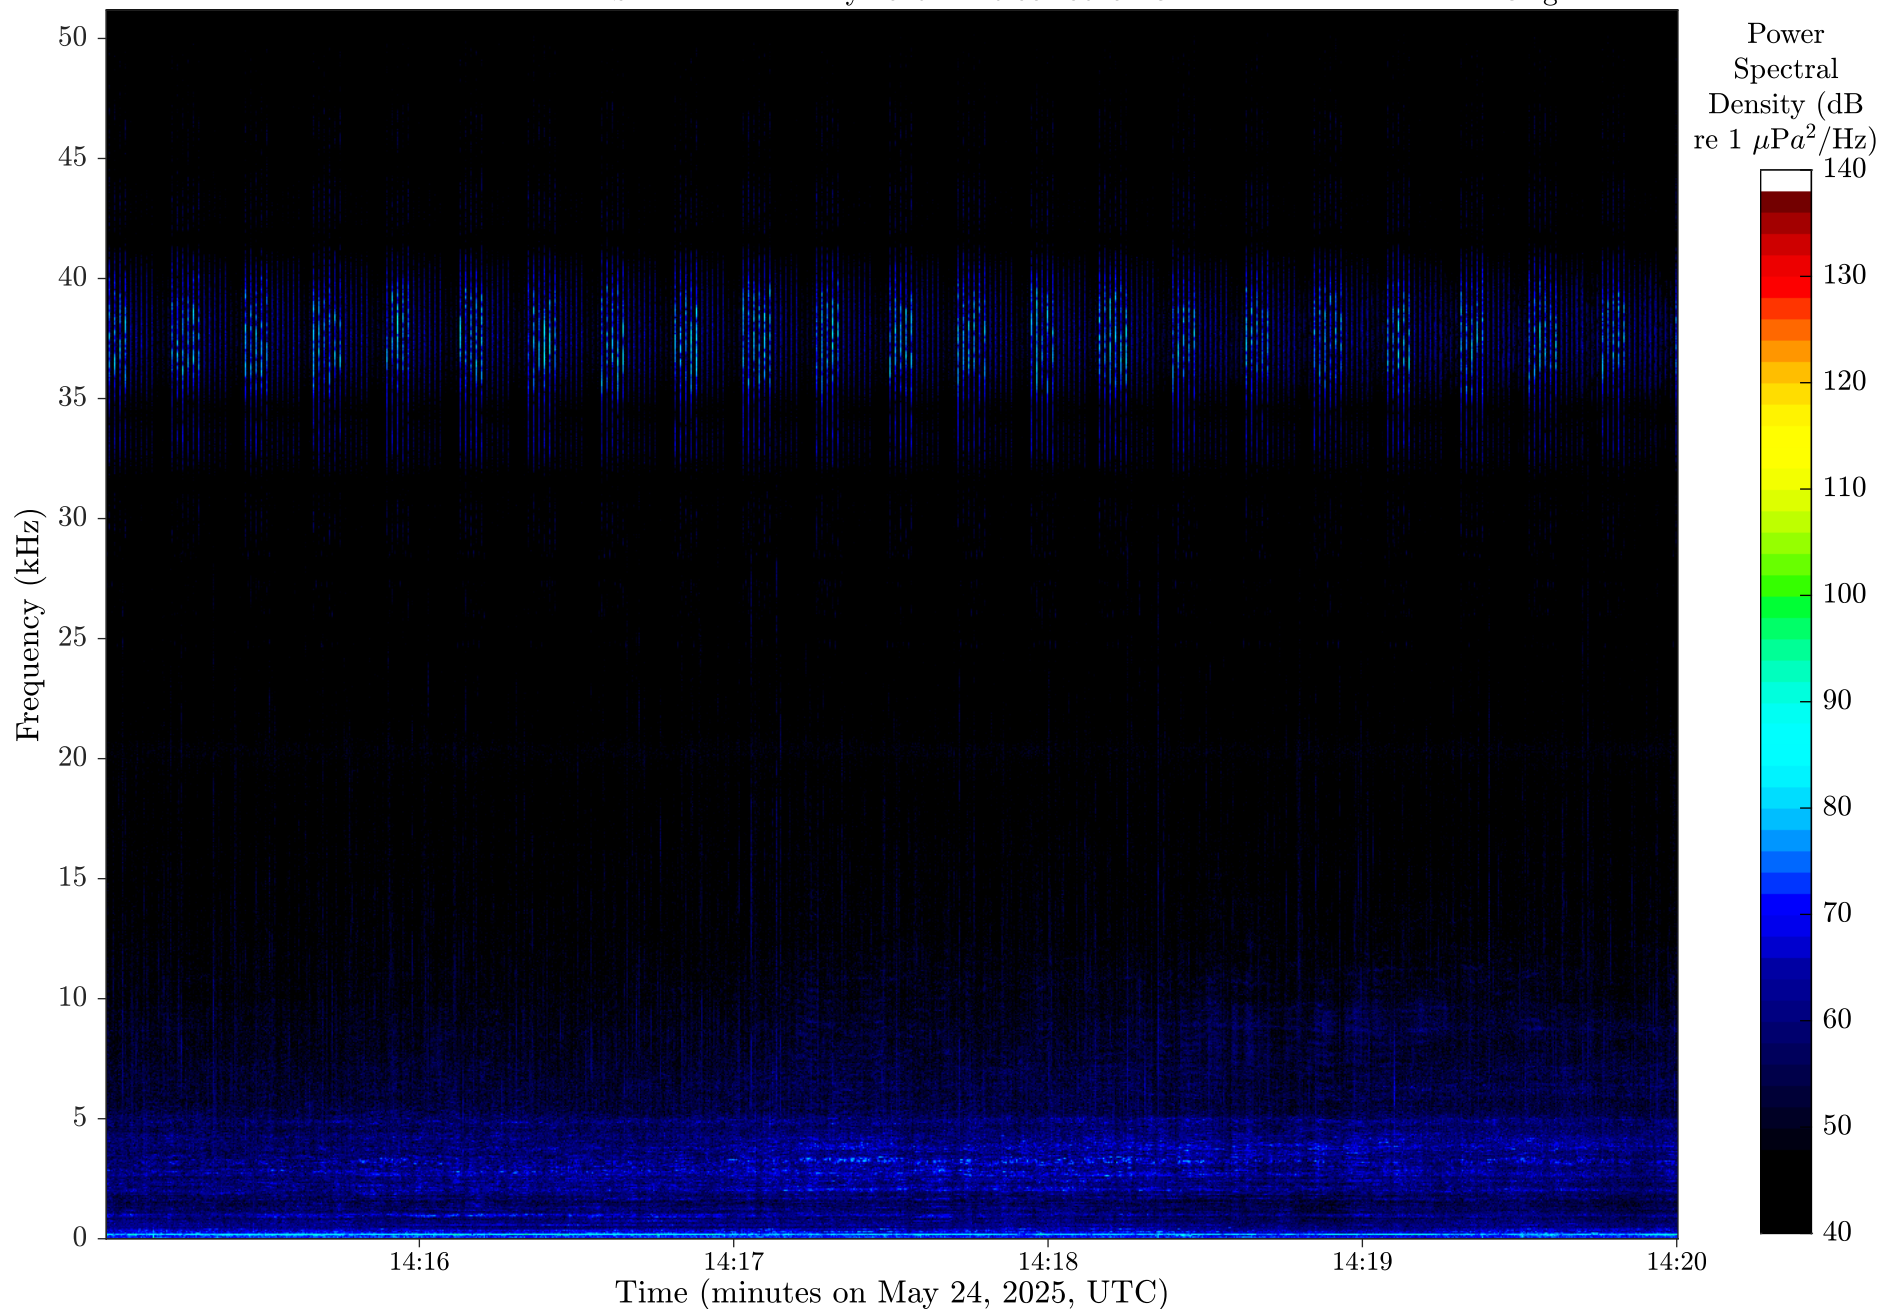


Comments: 31.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:33:04 UTC

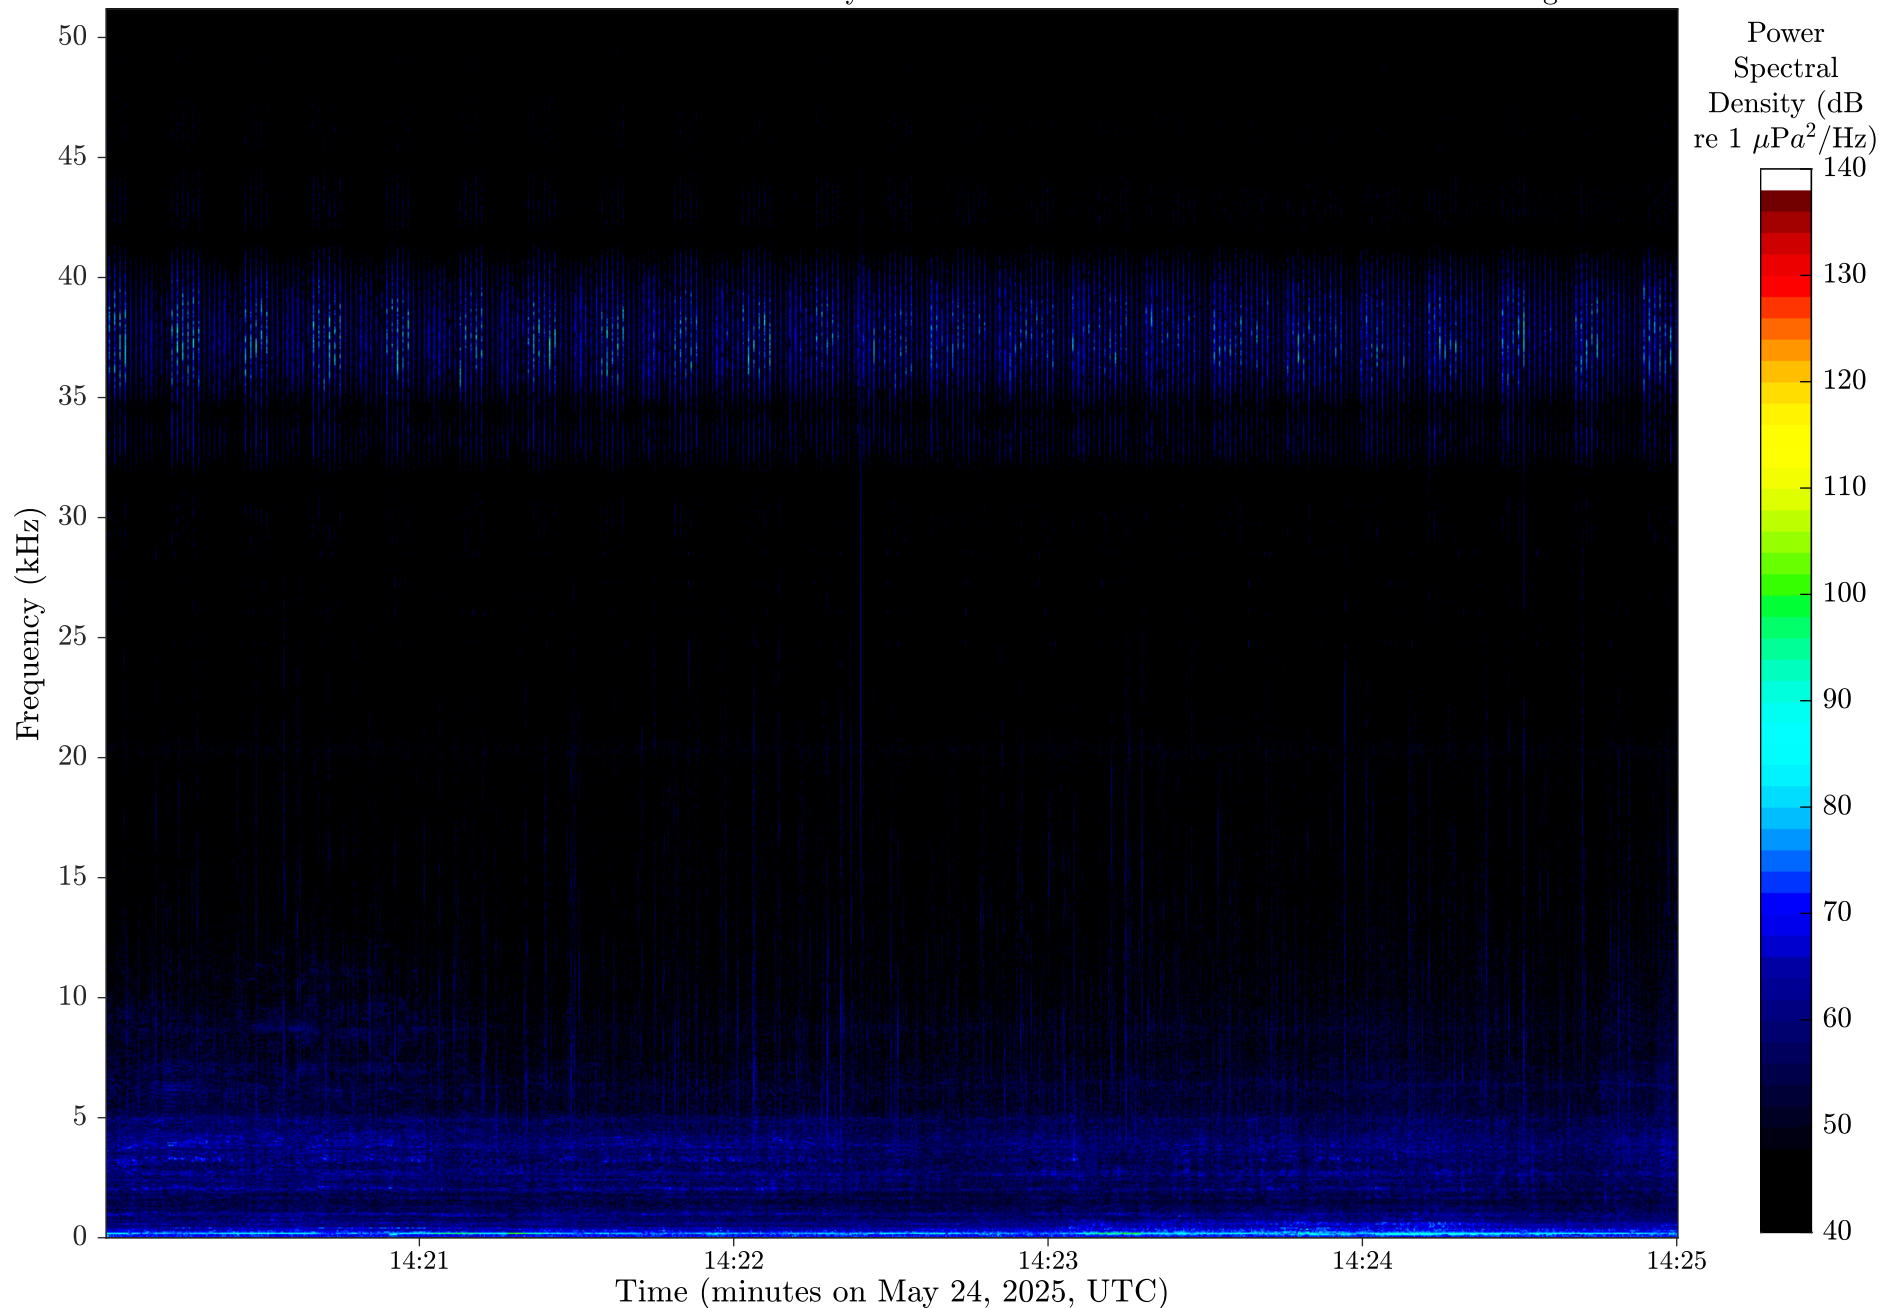


Comments: 30.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:33:11 UTC

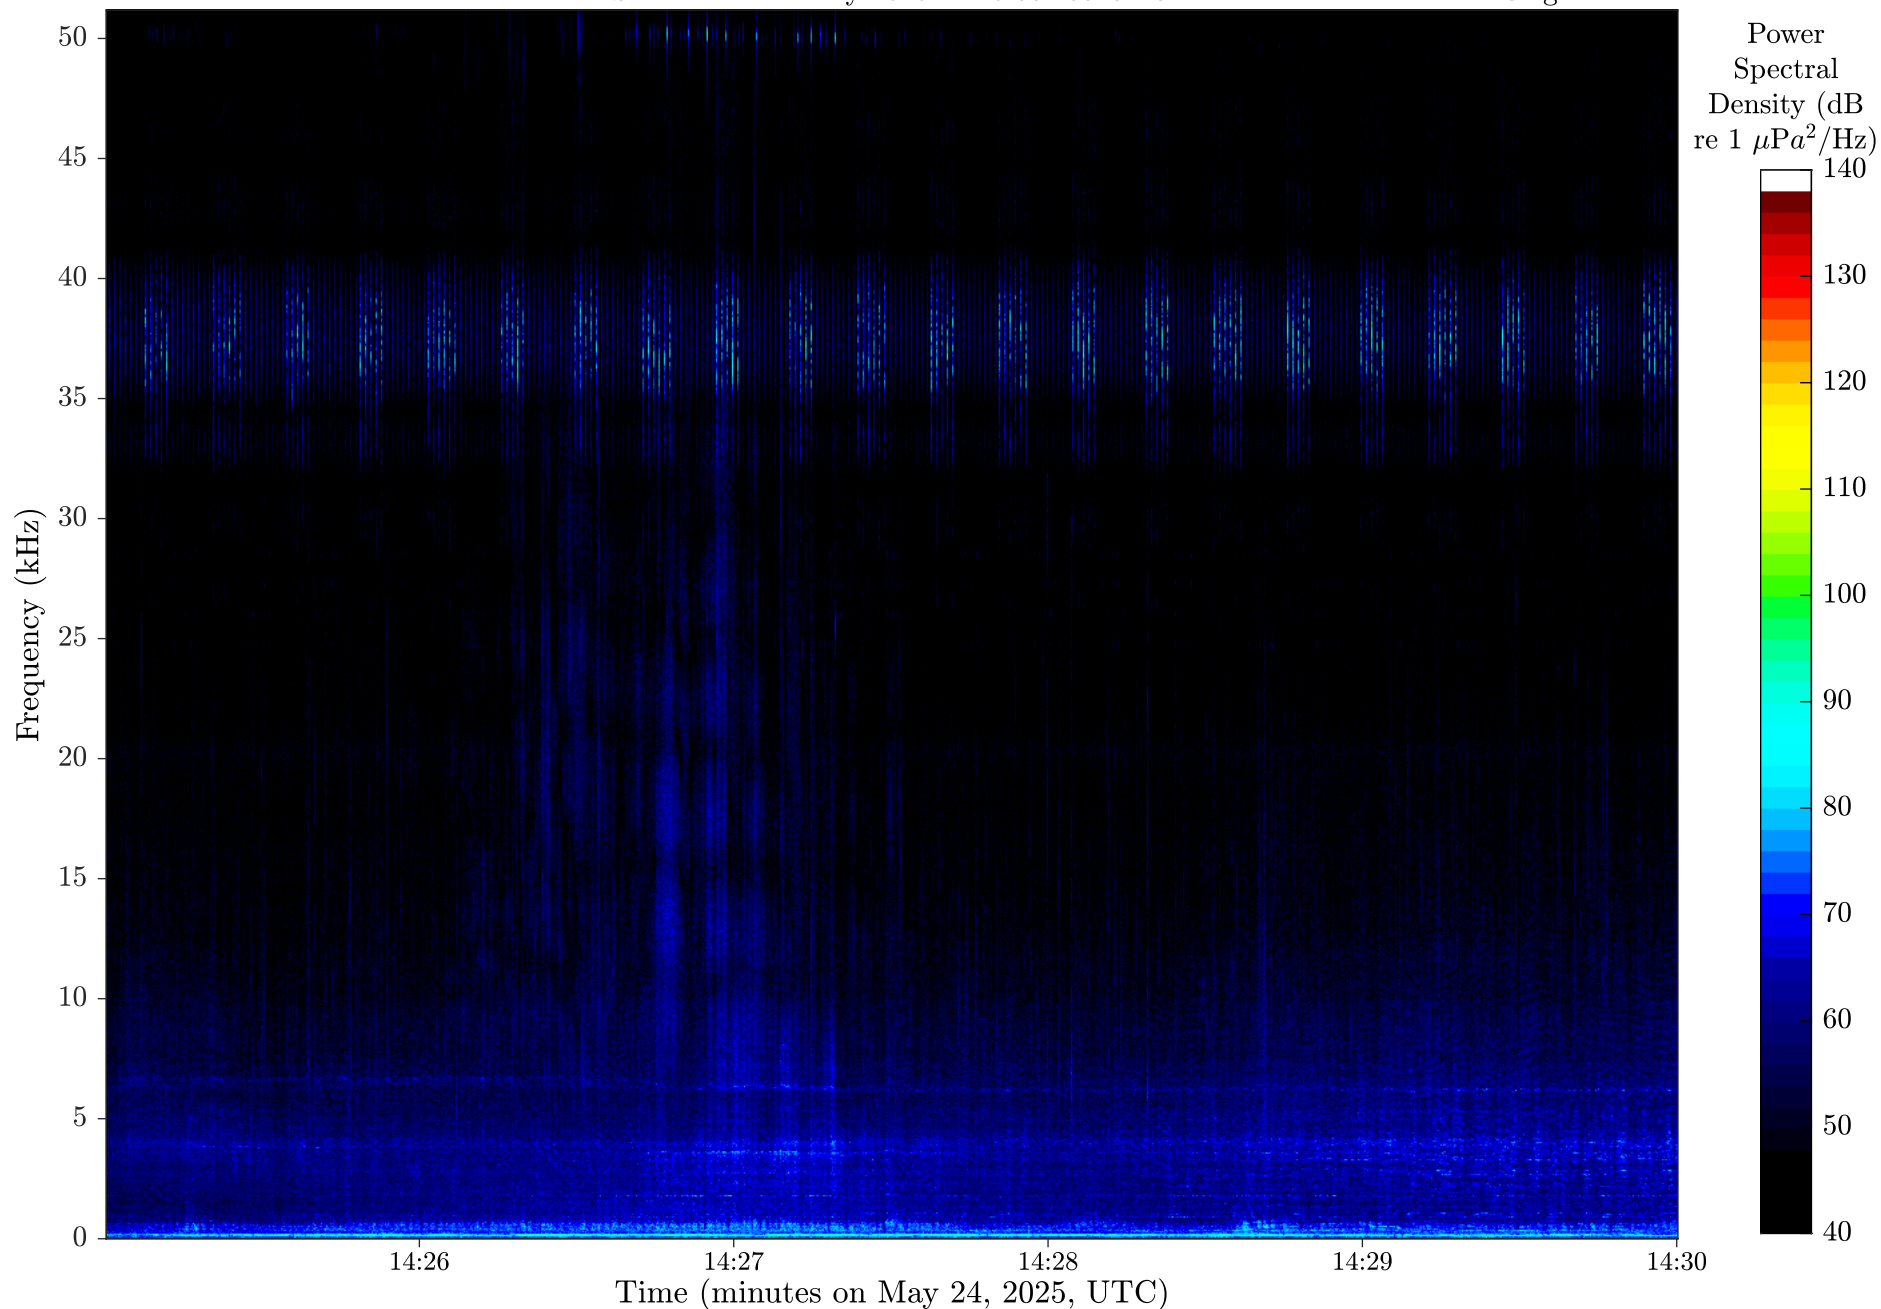


Comments: 20.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:33:18 UTC

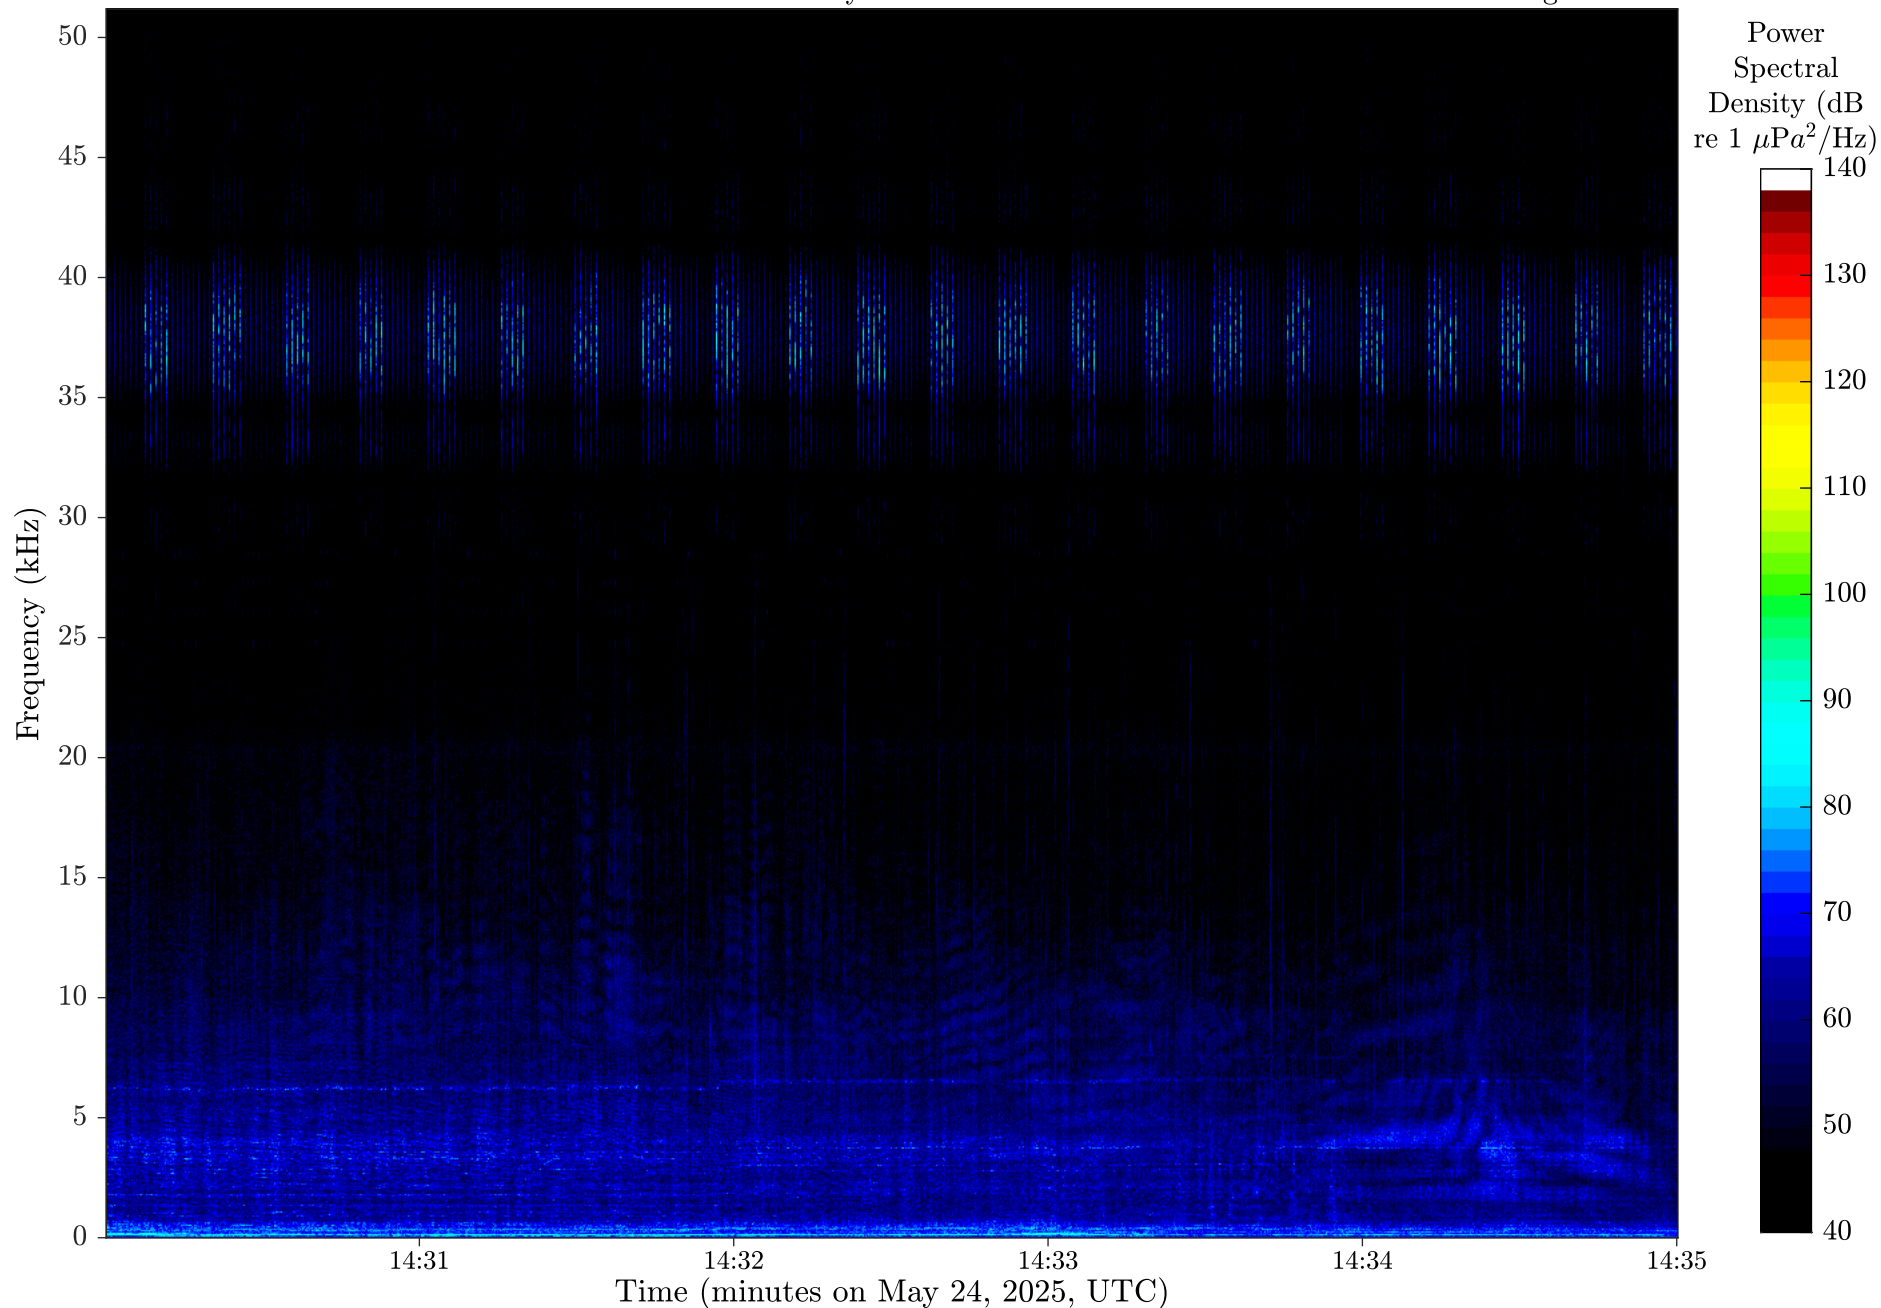

Comments: 27.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:33:25 UTC

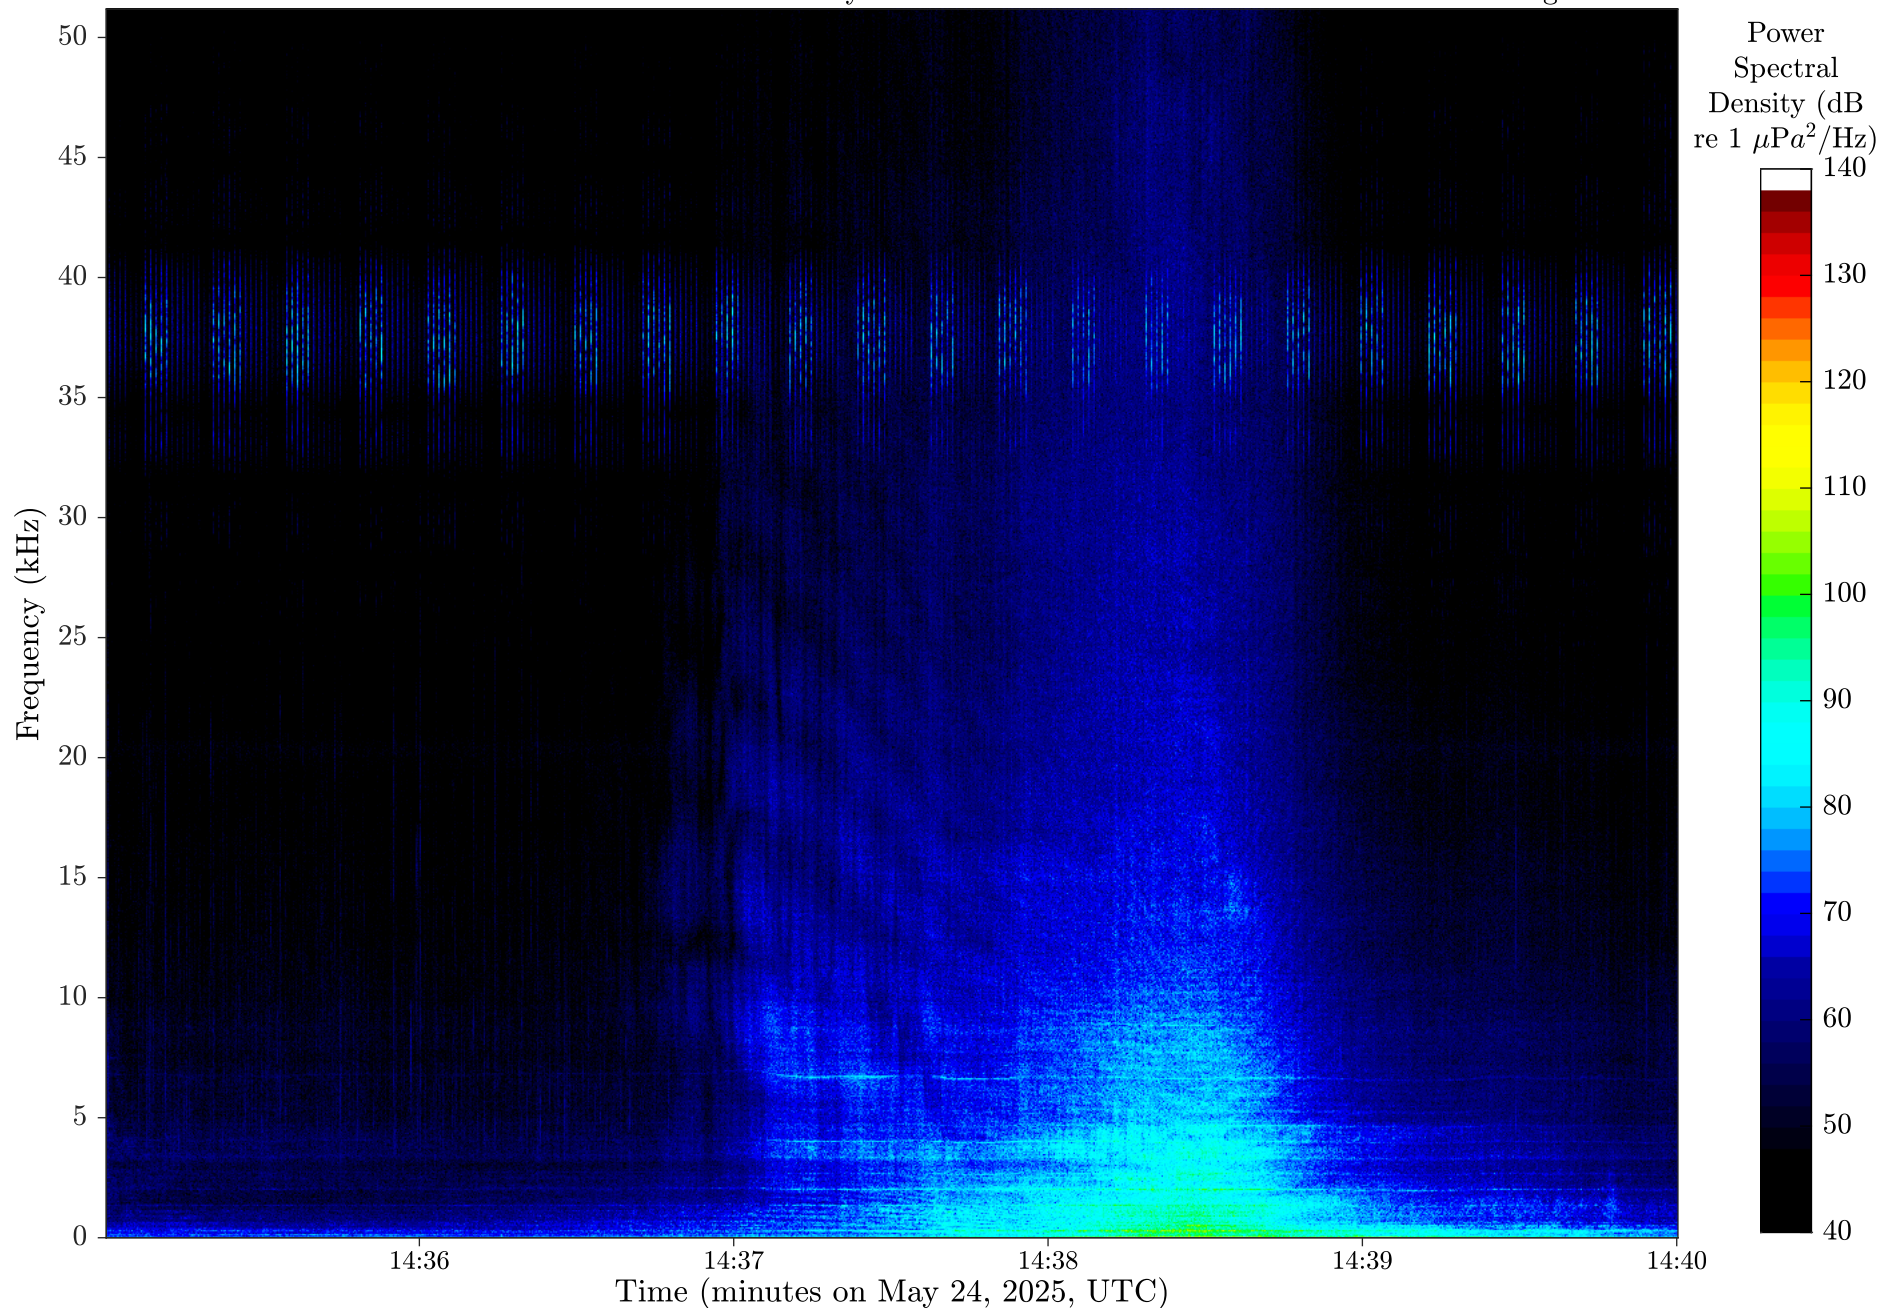

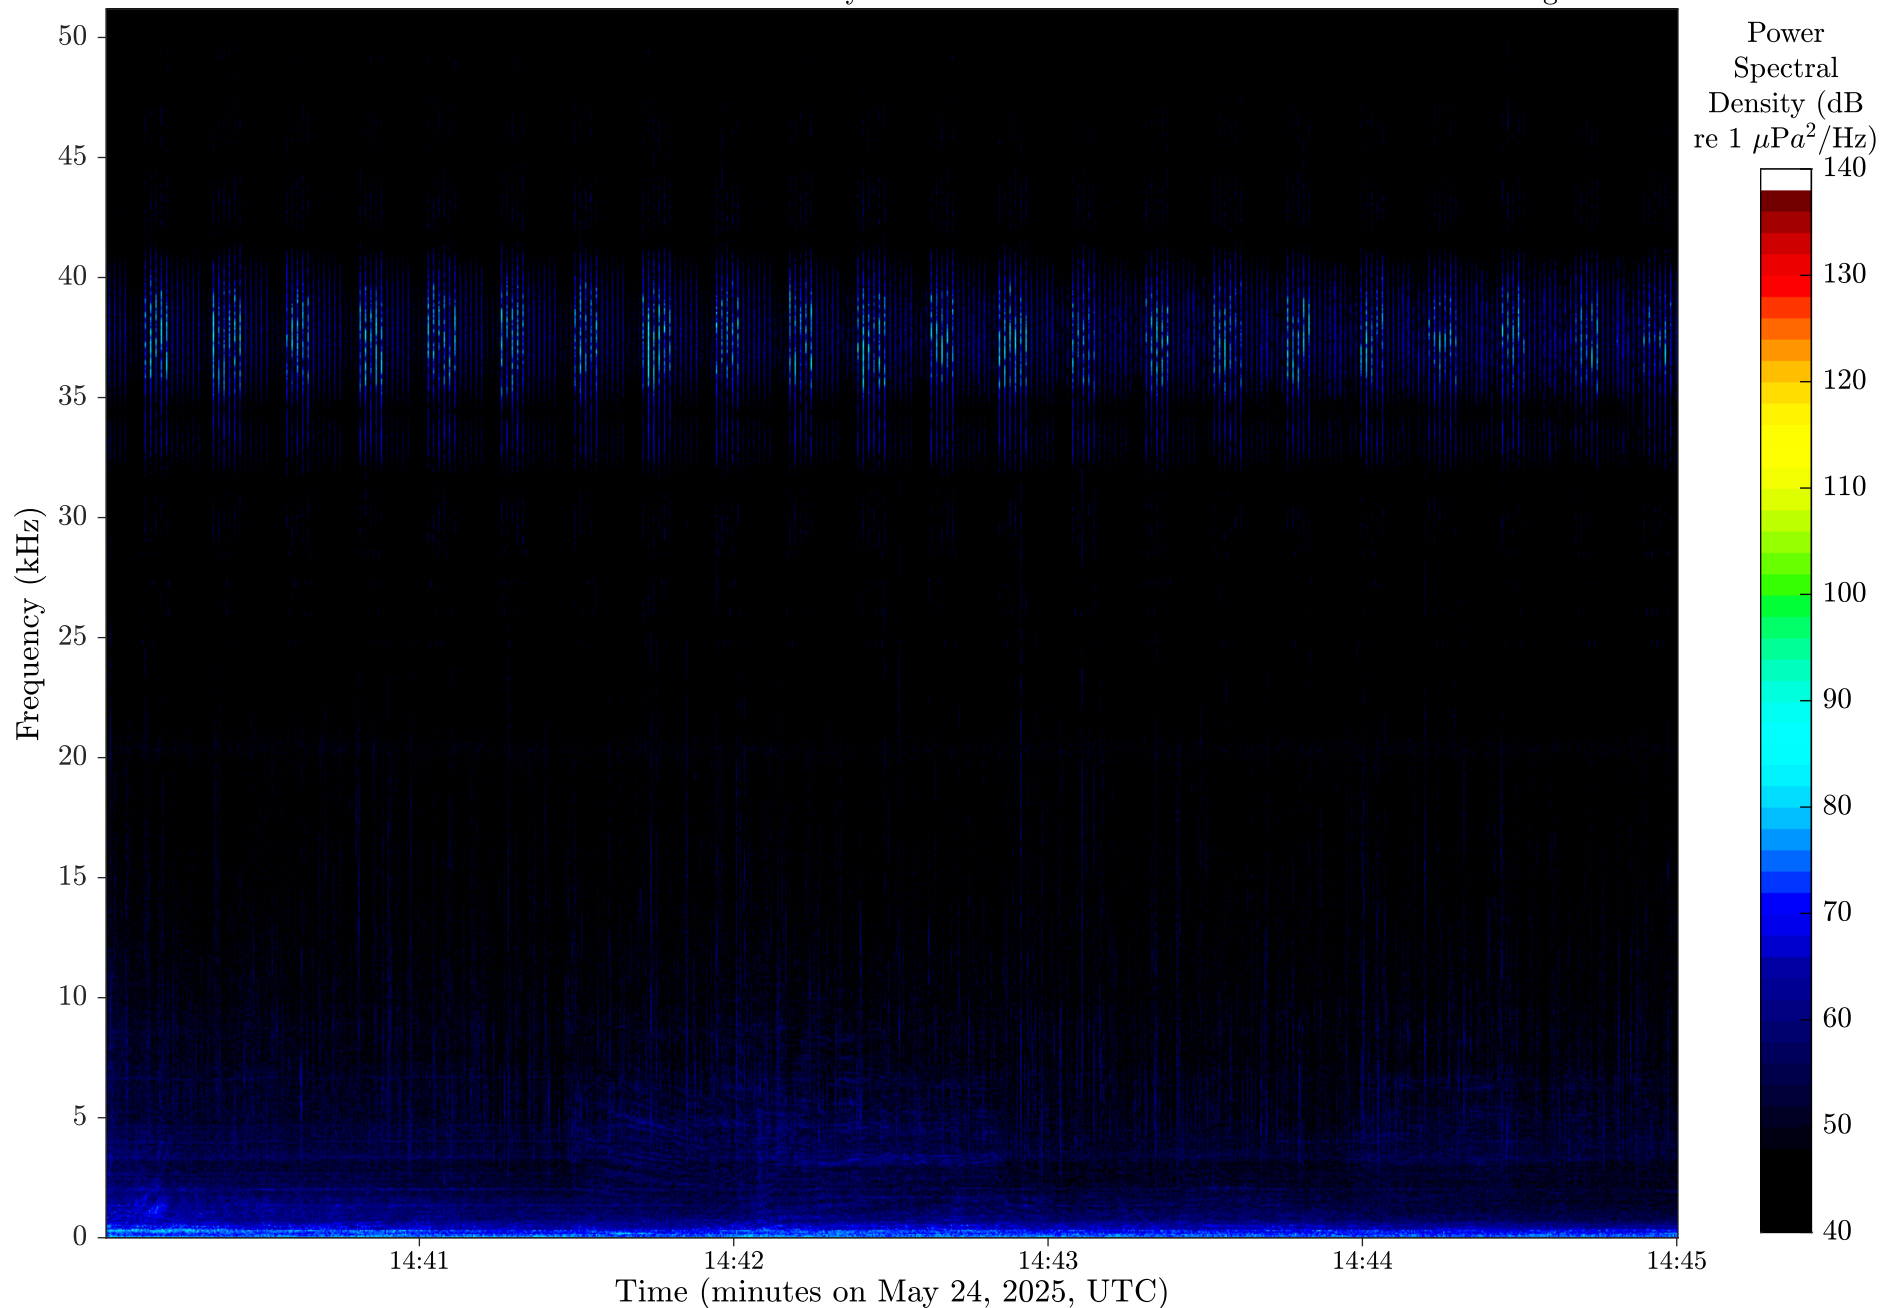


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:33:39 UTC

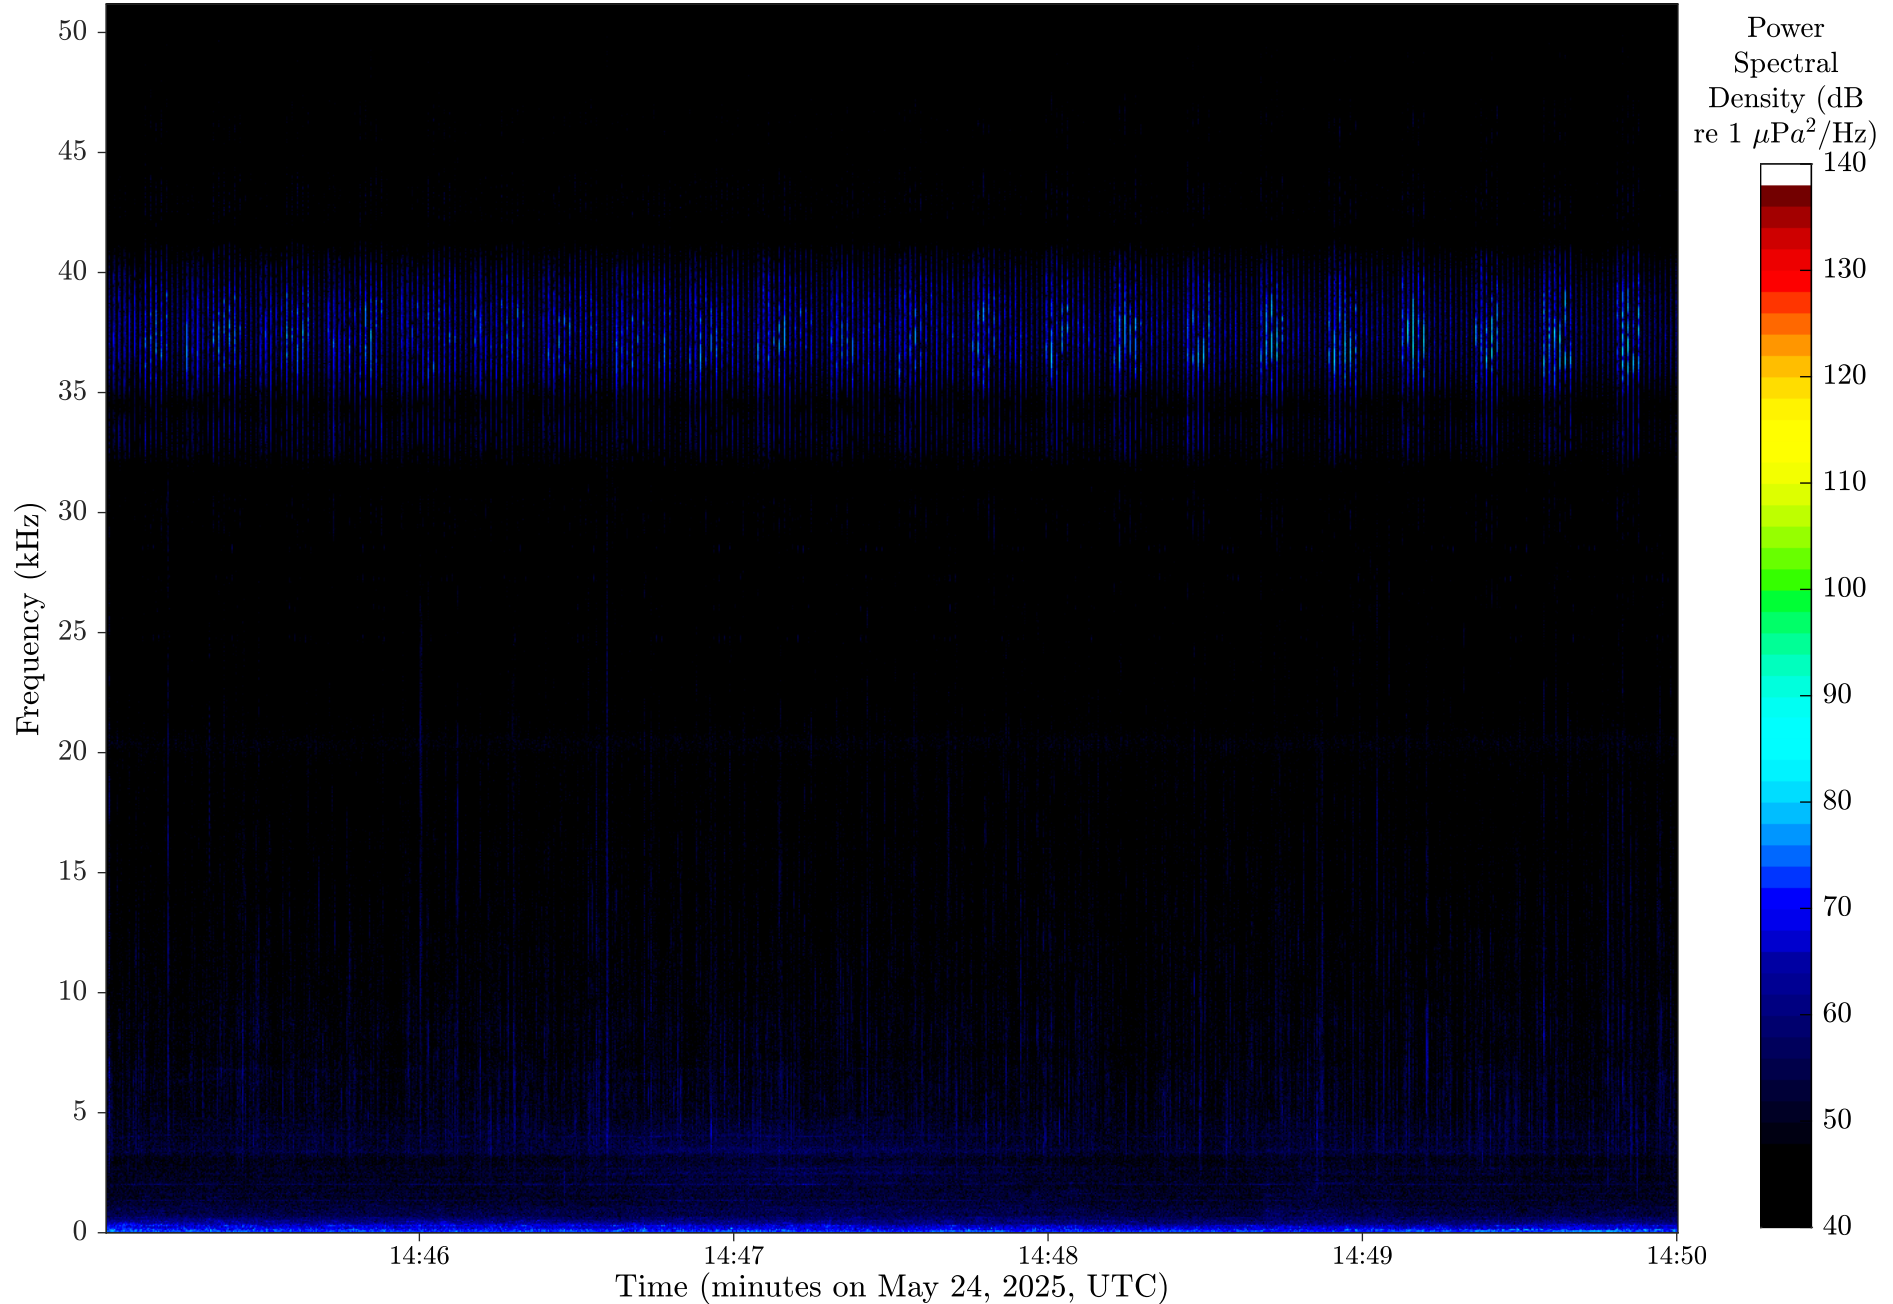


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:33:47 UTC

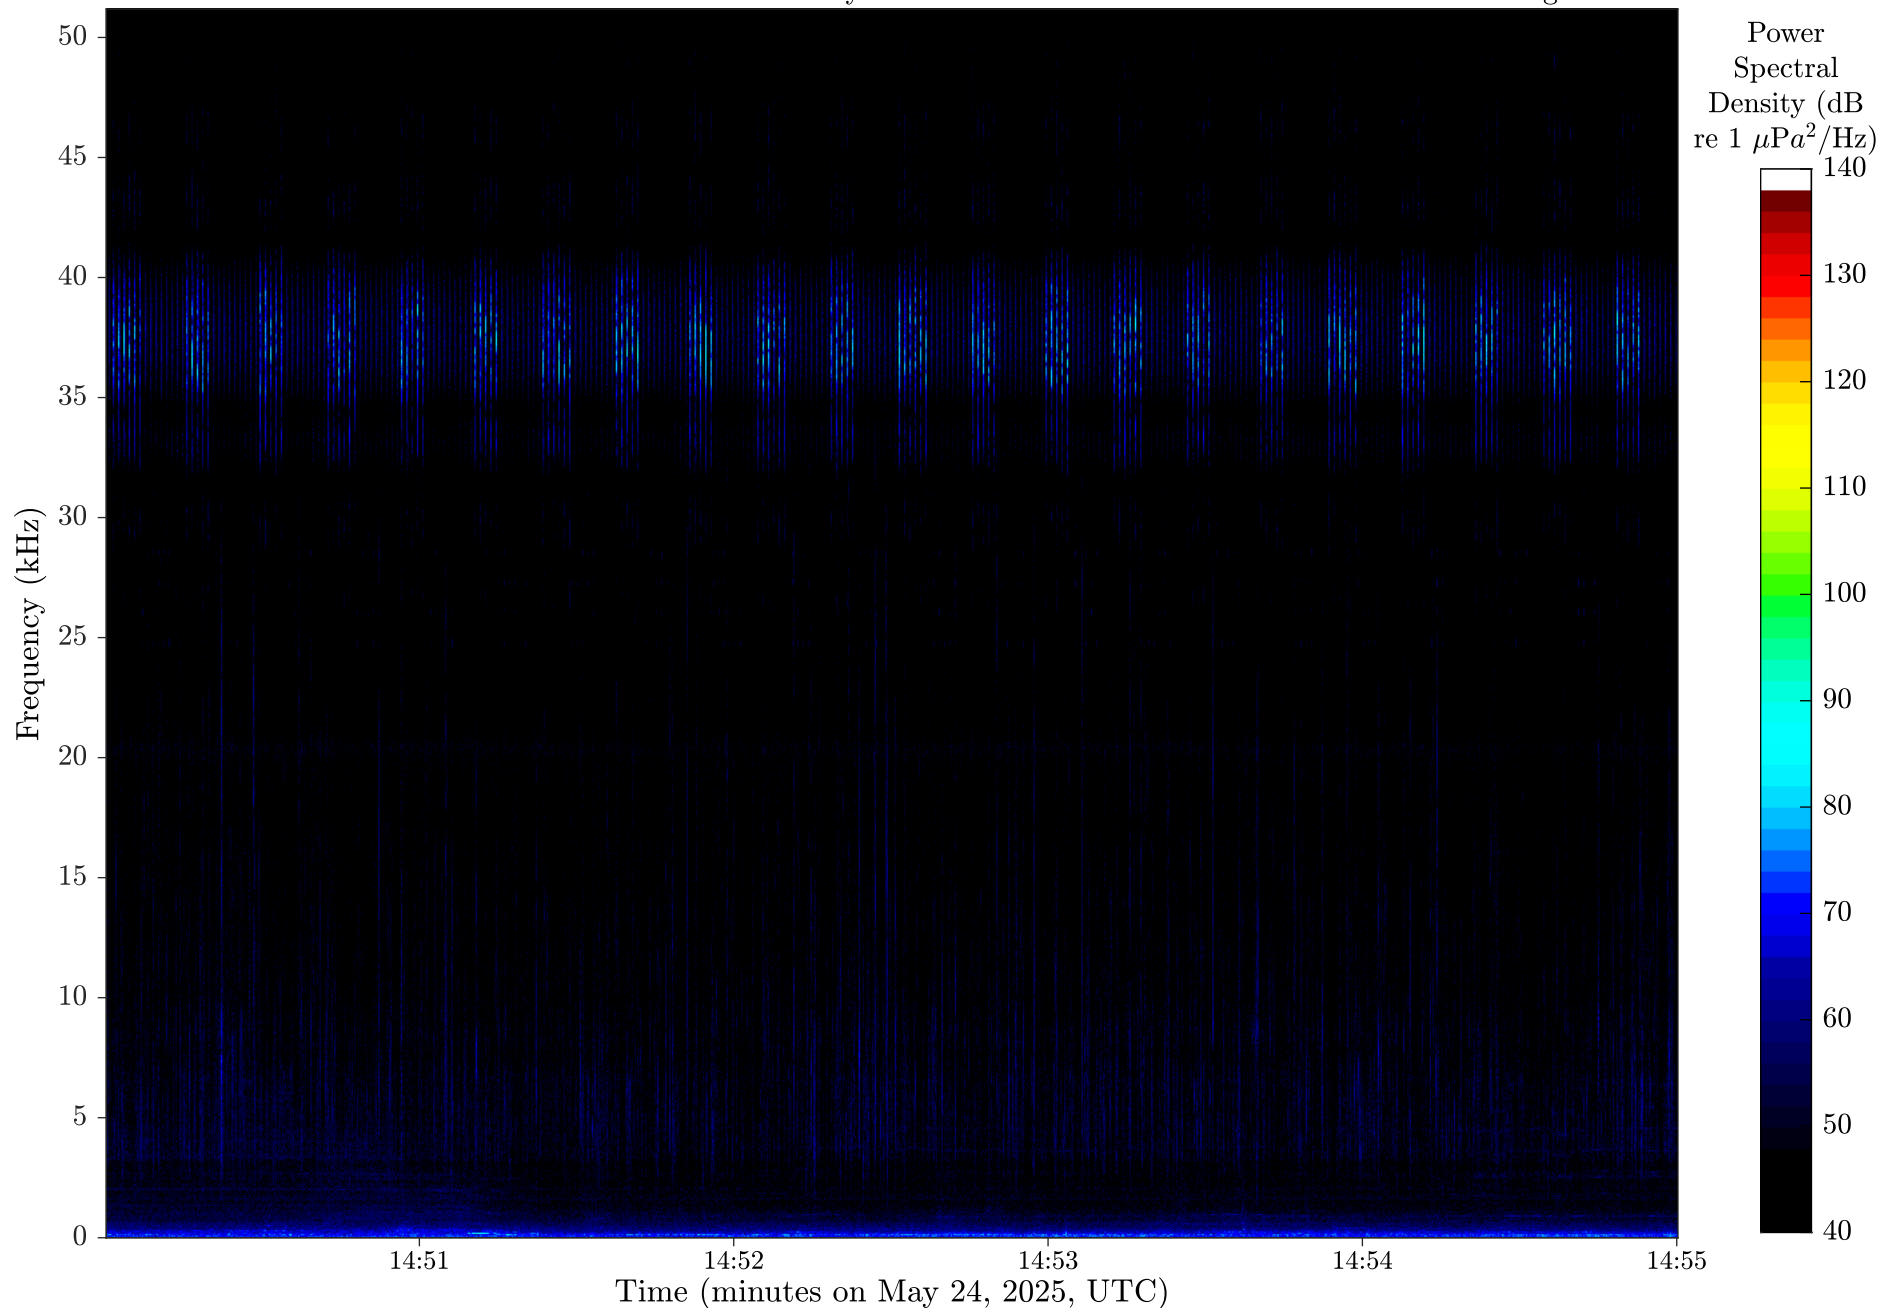

Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:33:54 UTC

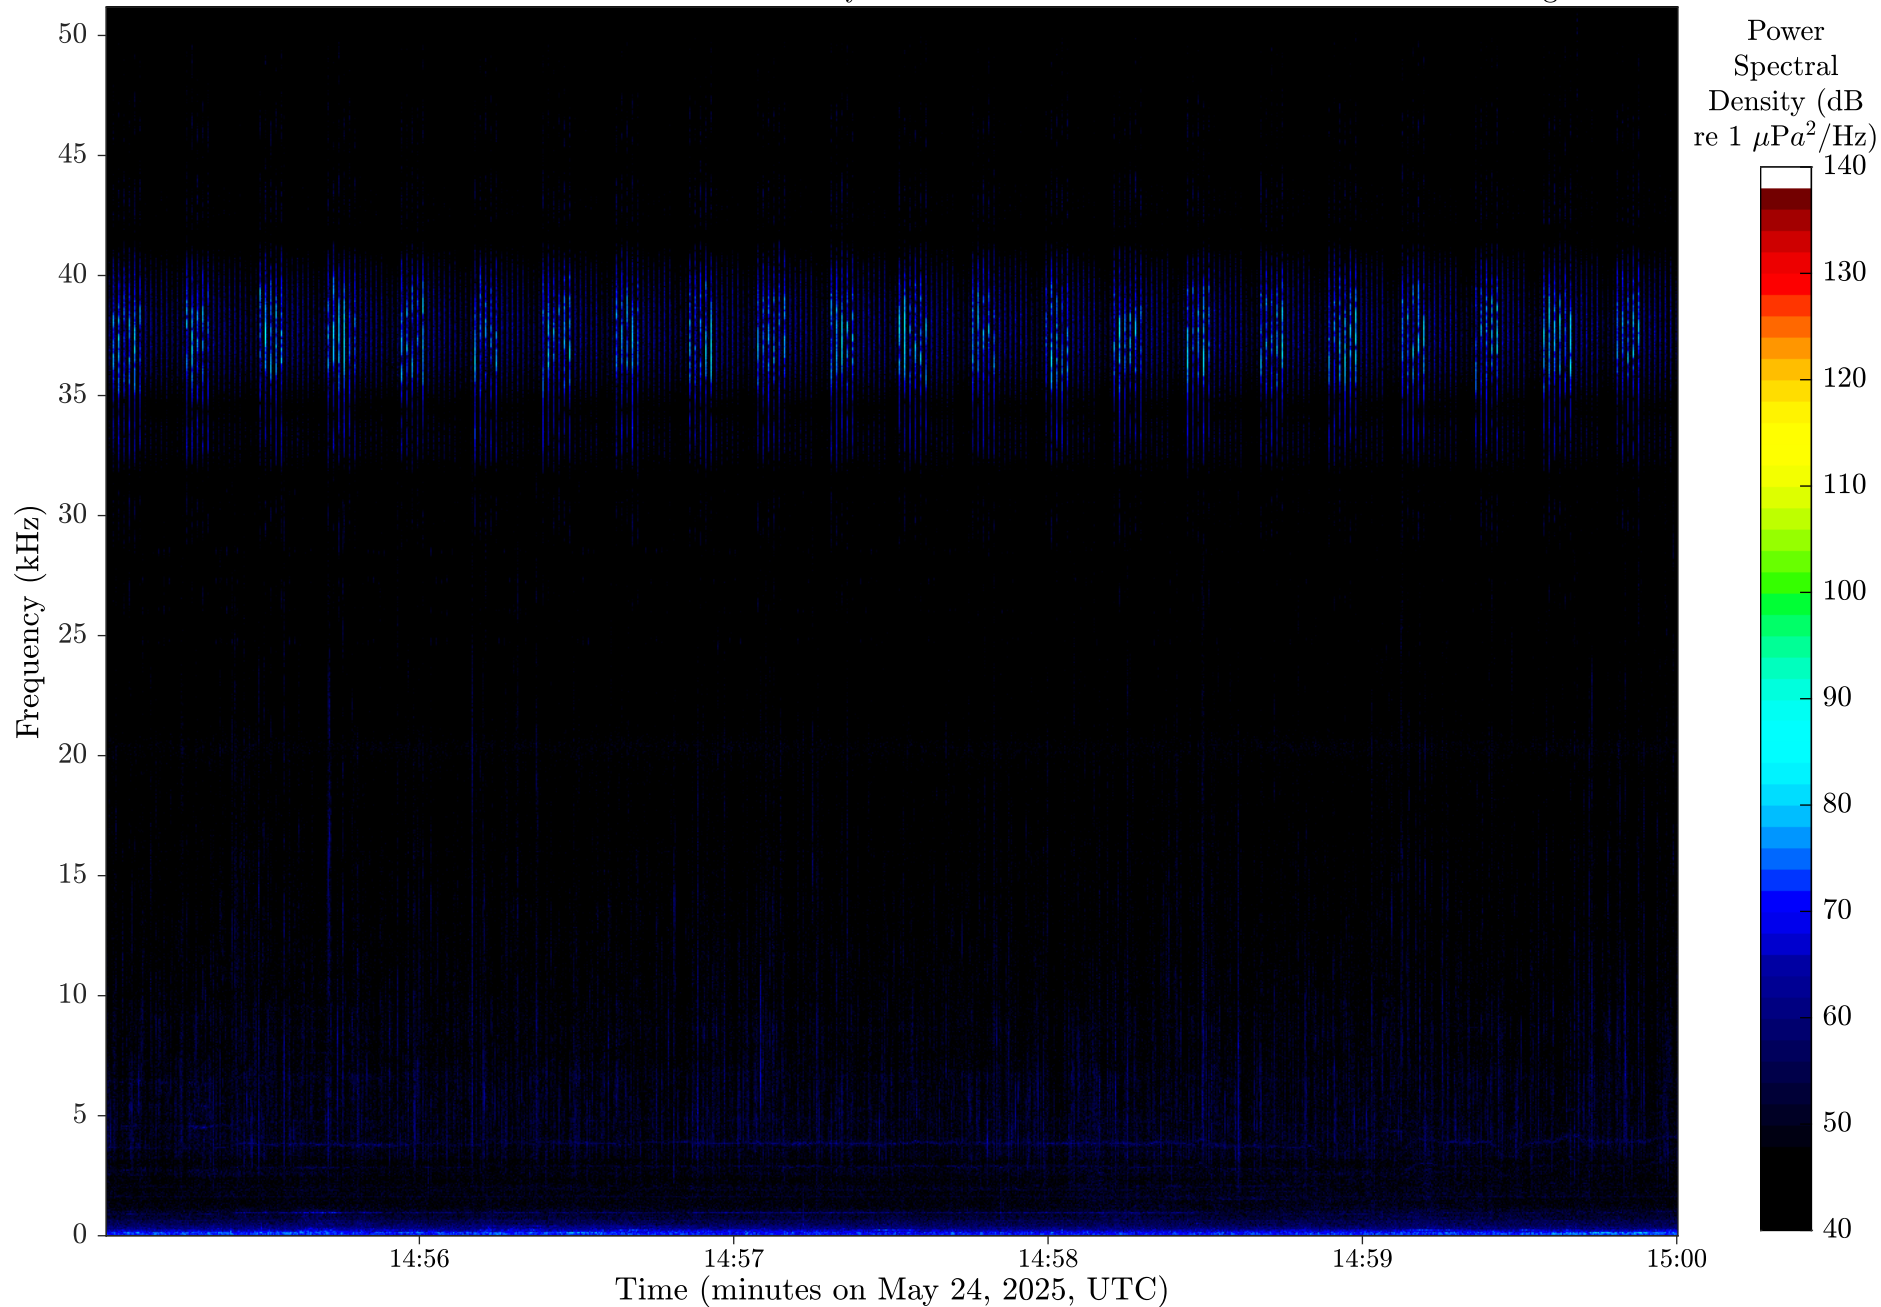

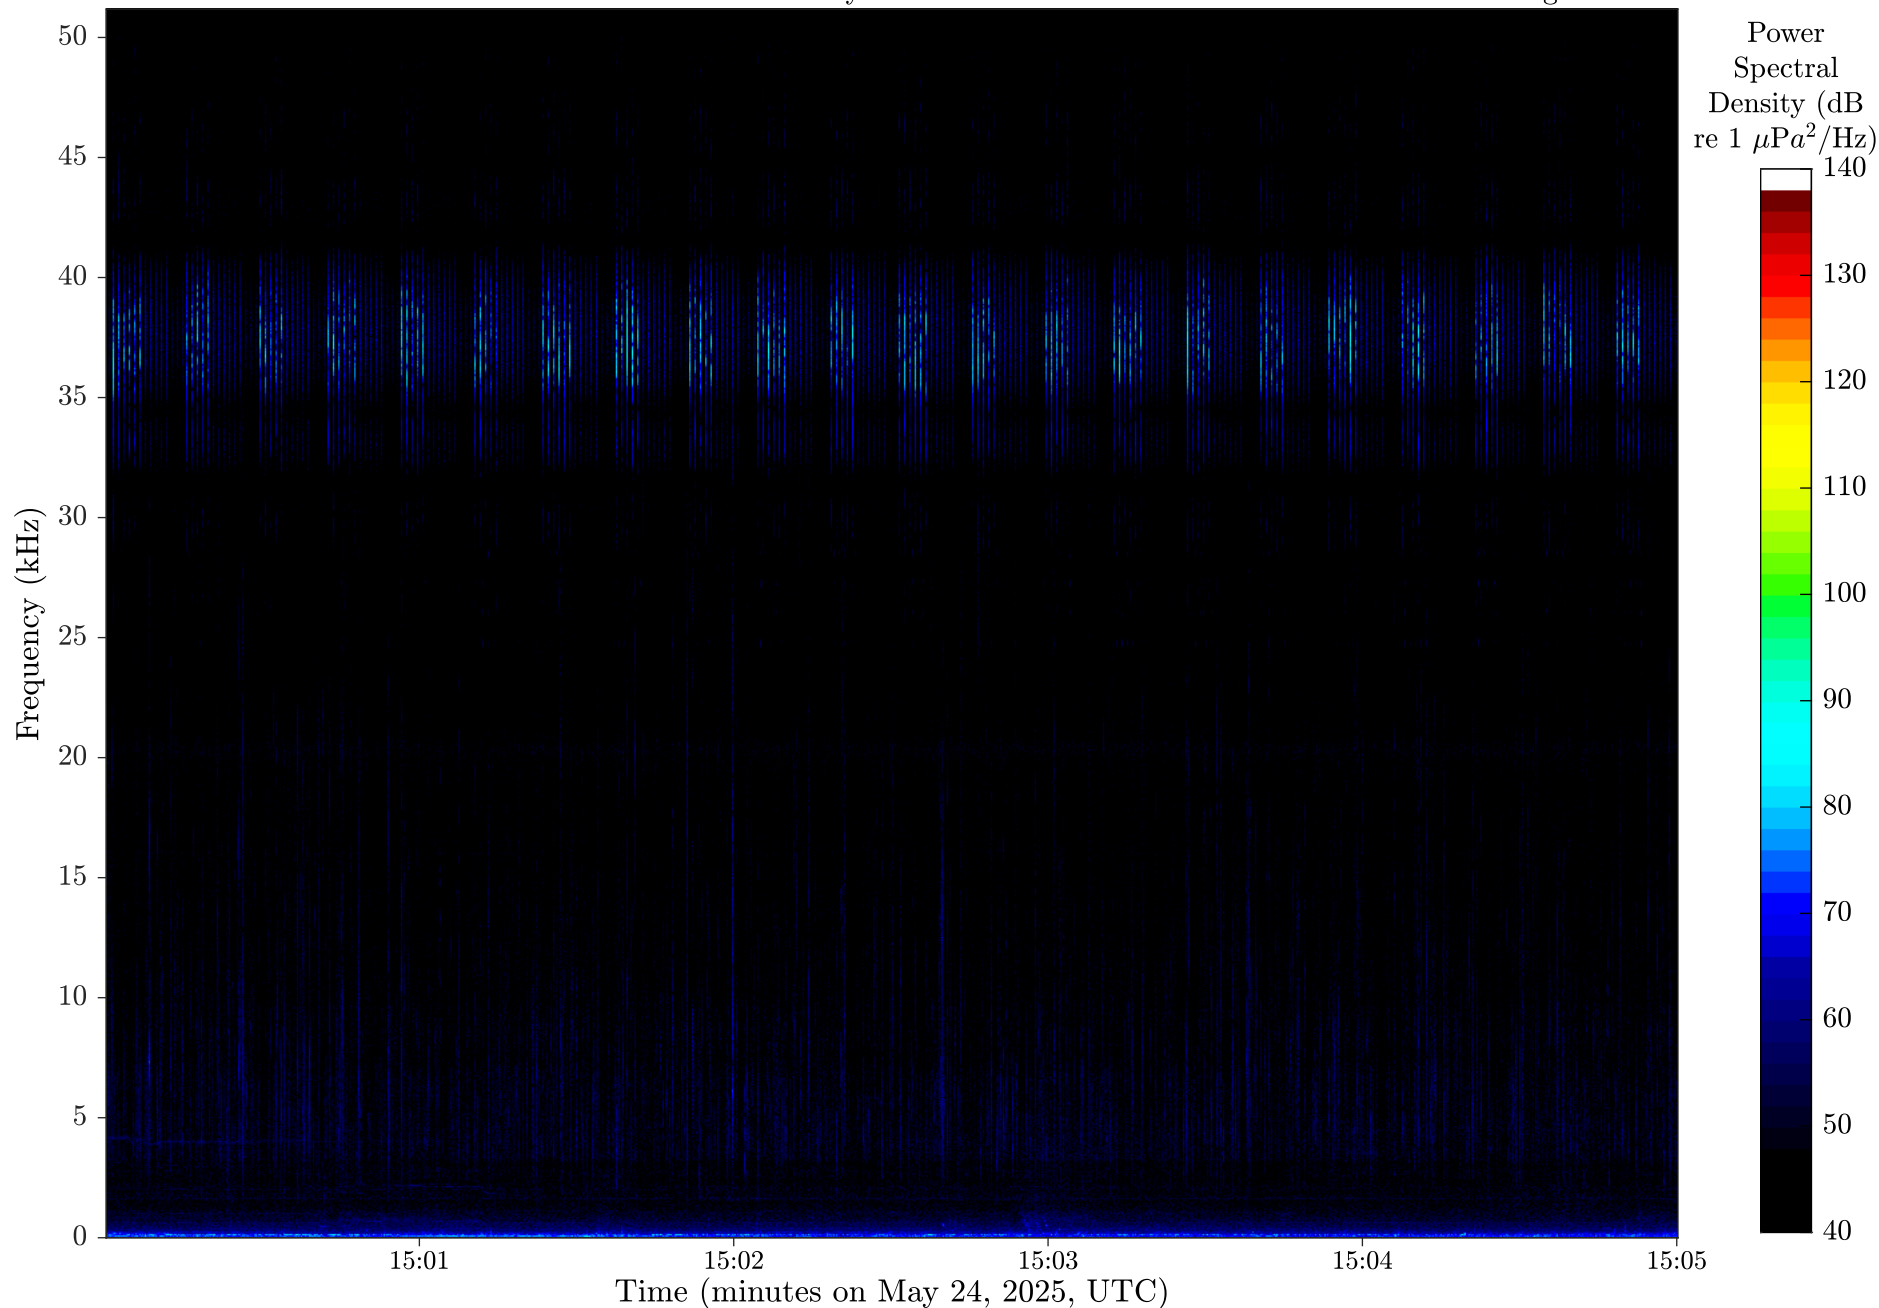


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:09 UTC

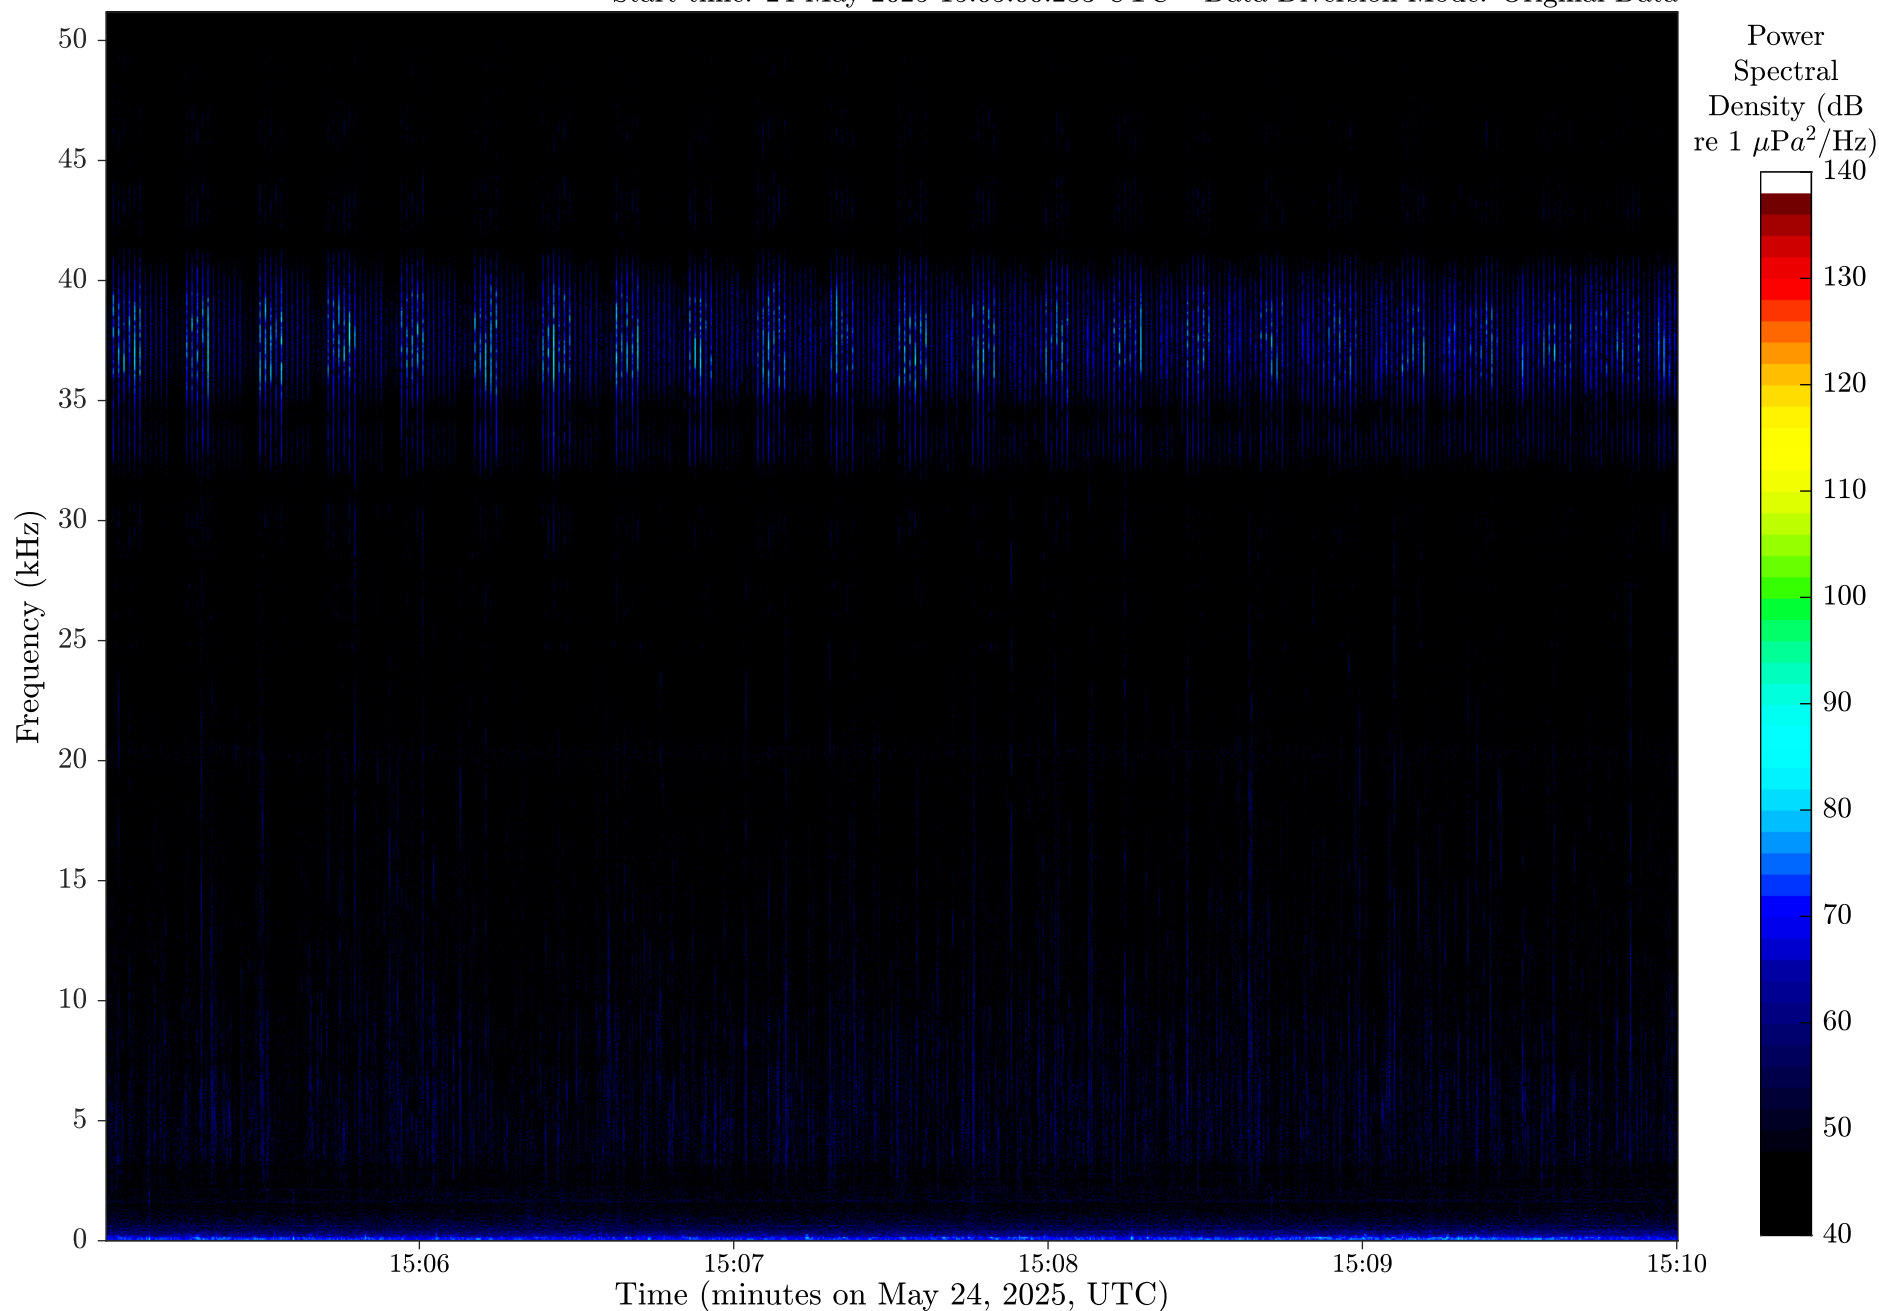


Comments: 32.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:16 UTC

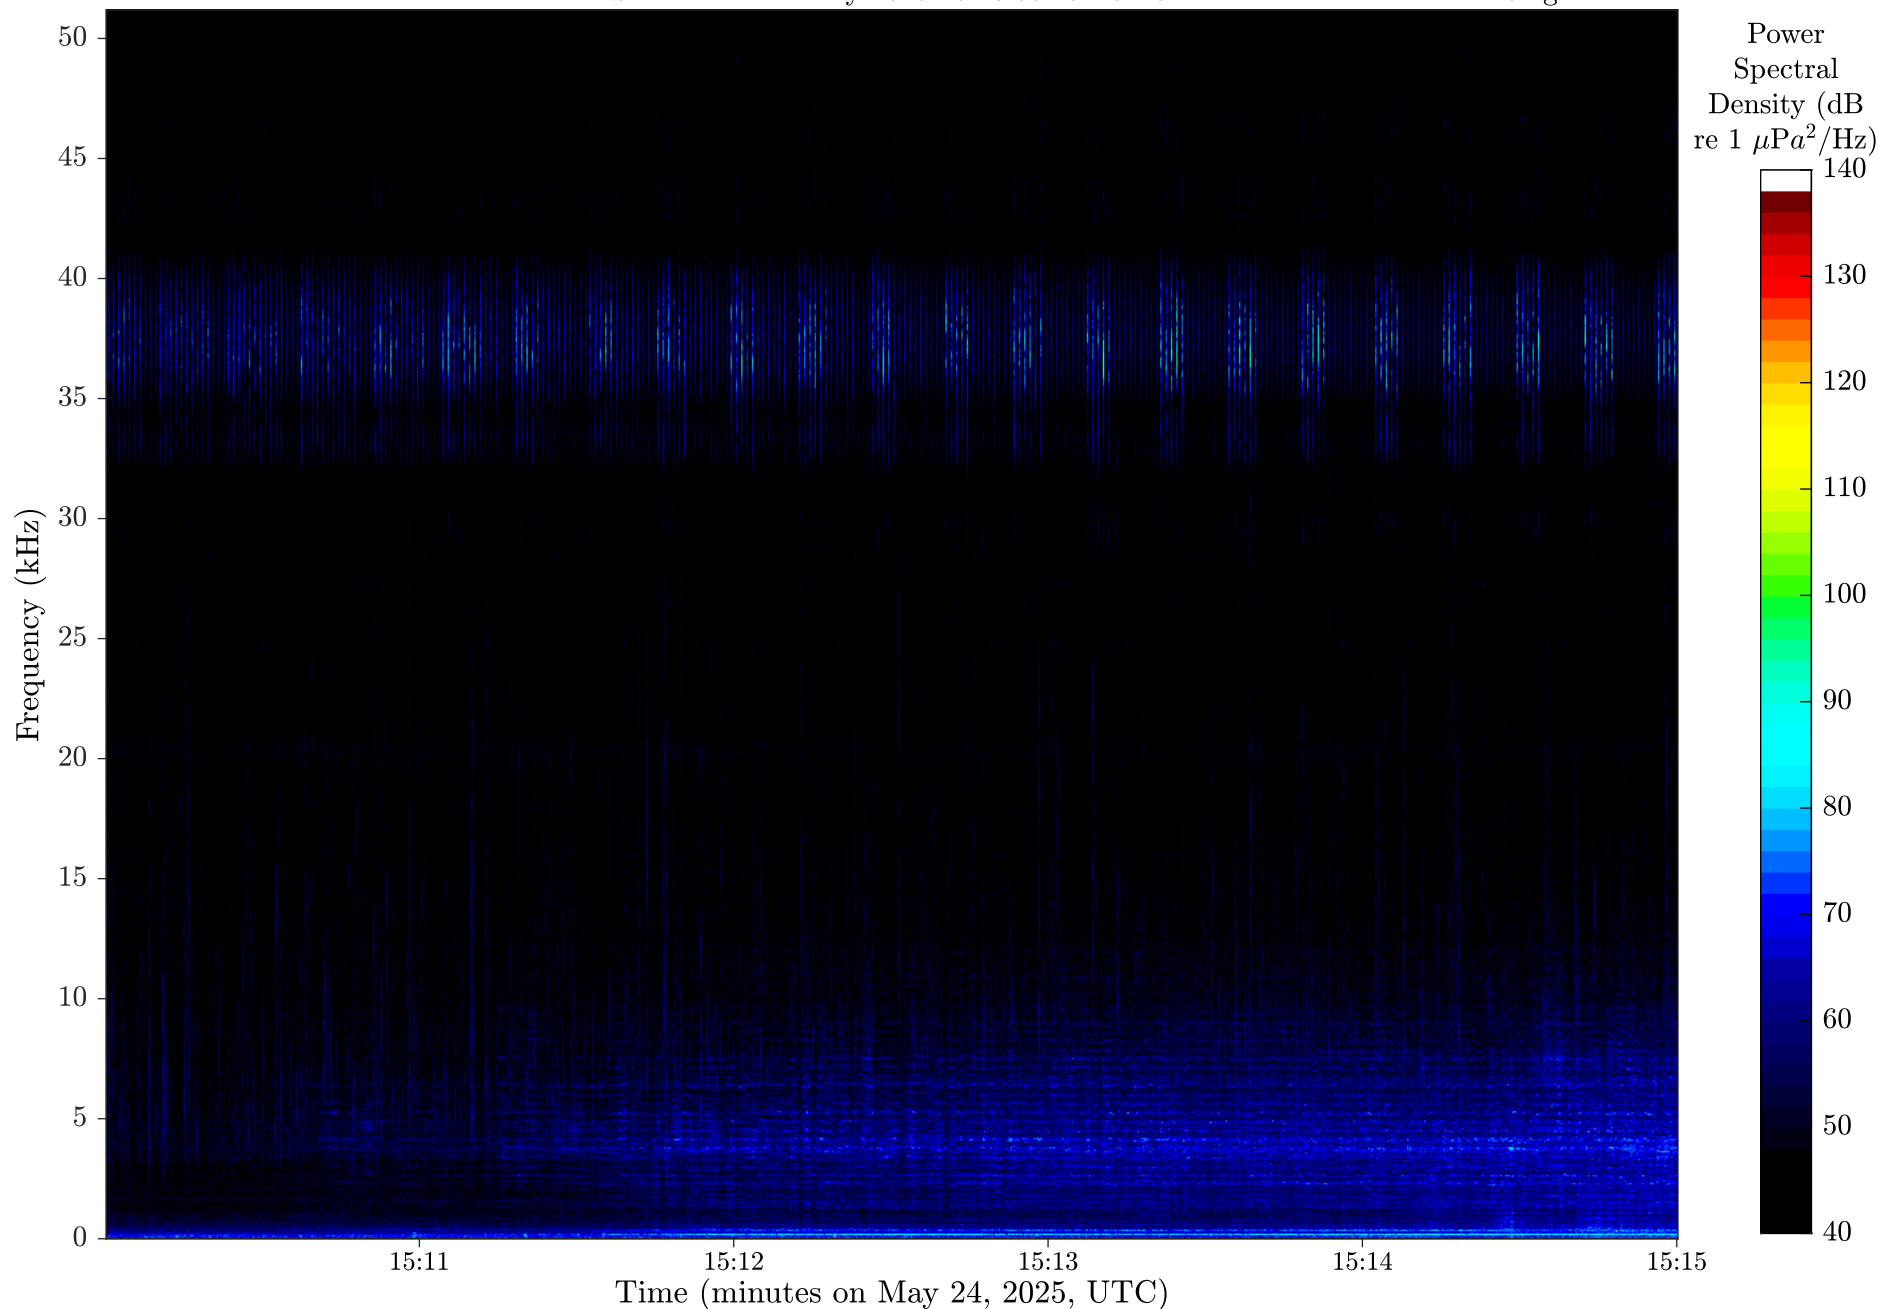


Comments: 31.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:24 UTC

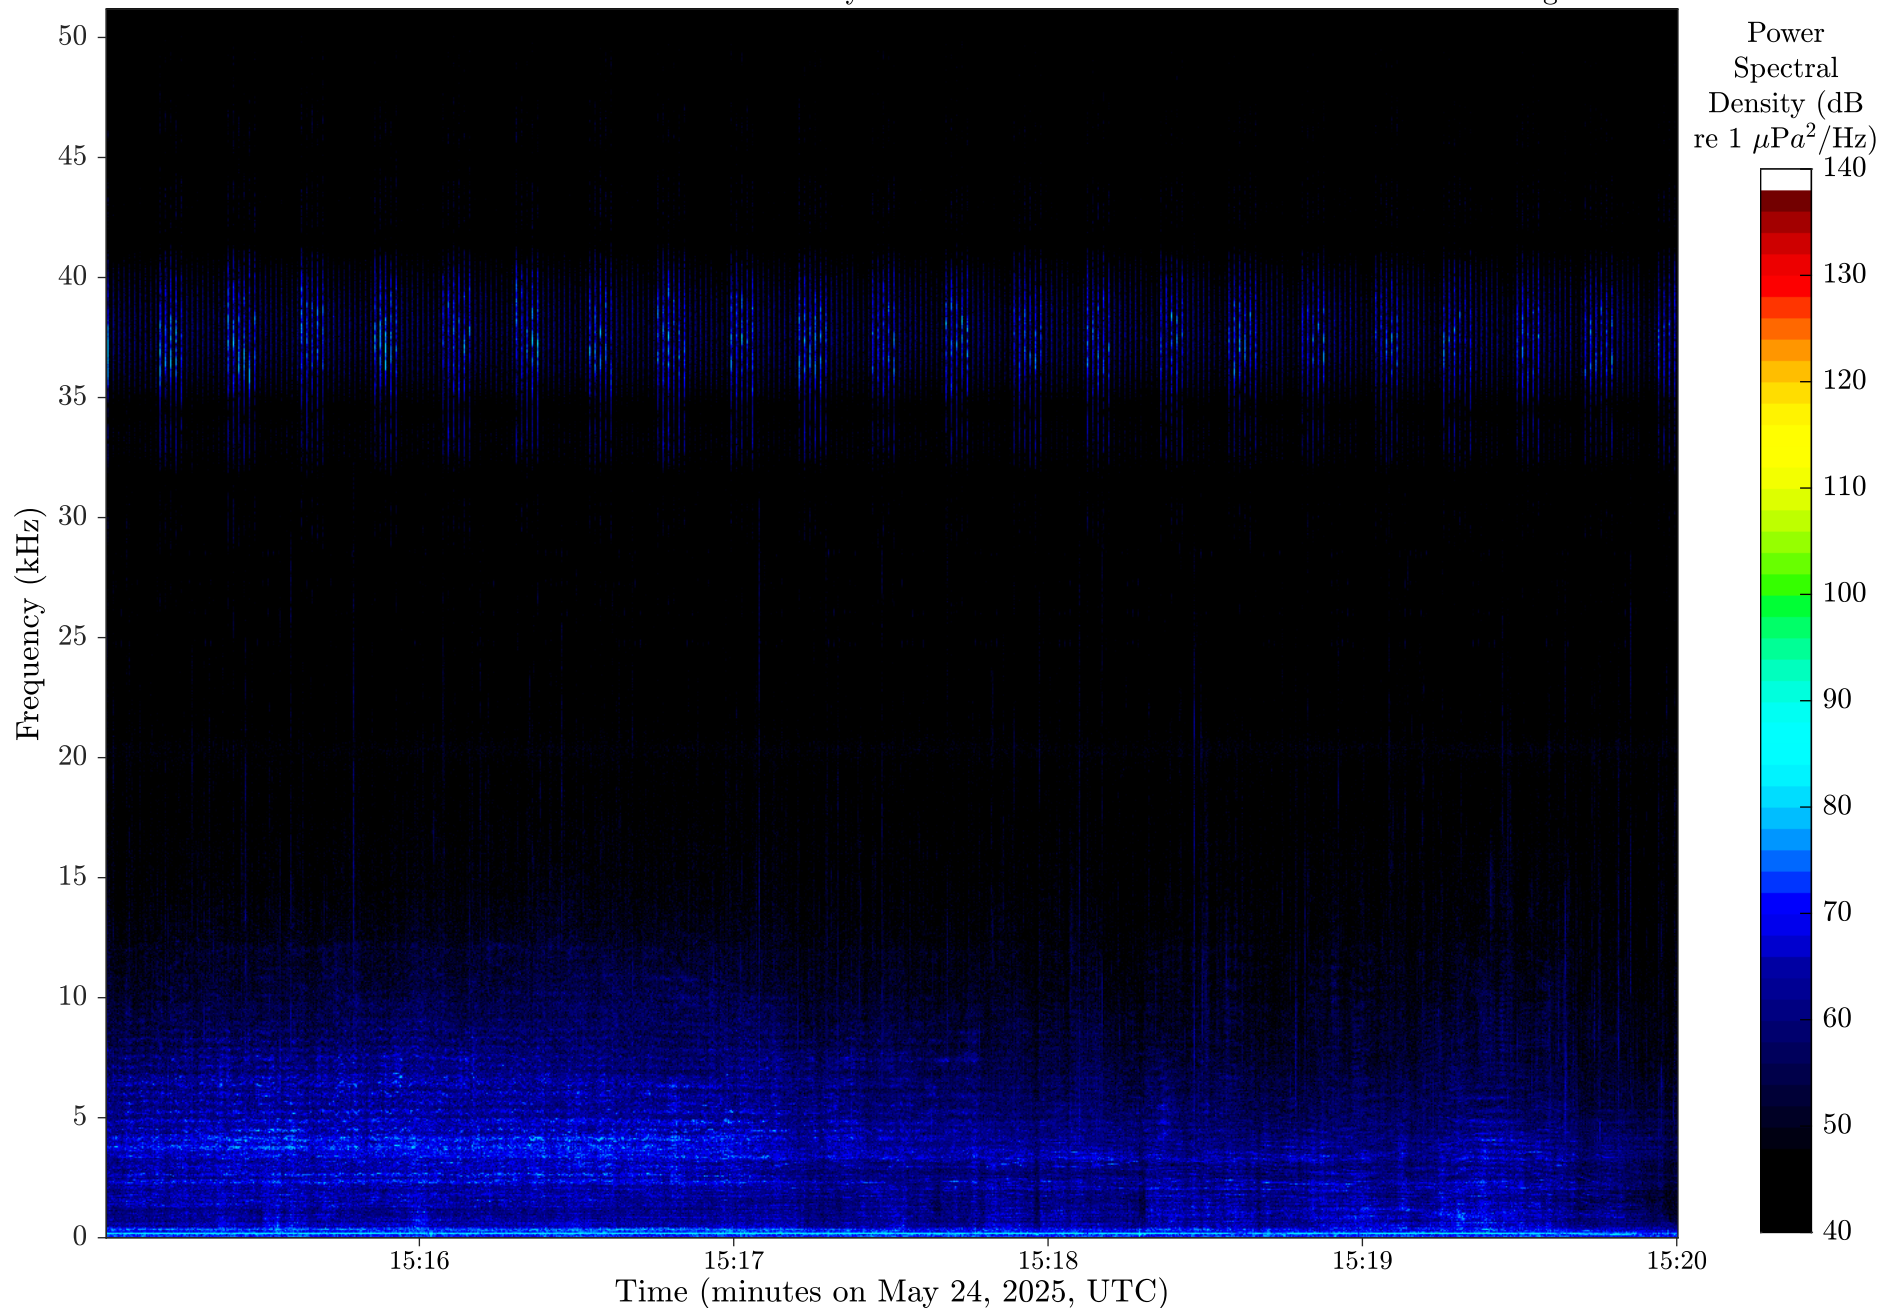


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:31 UTC

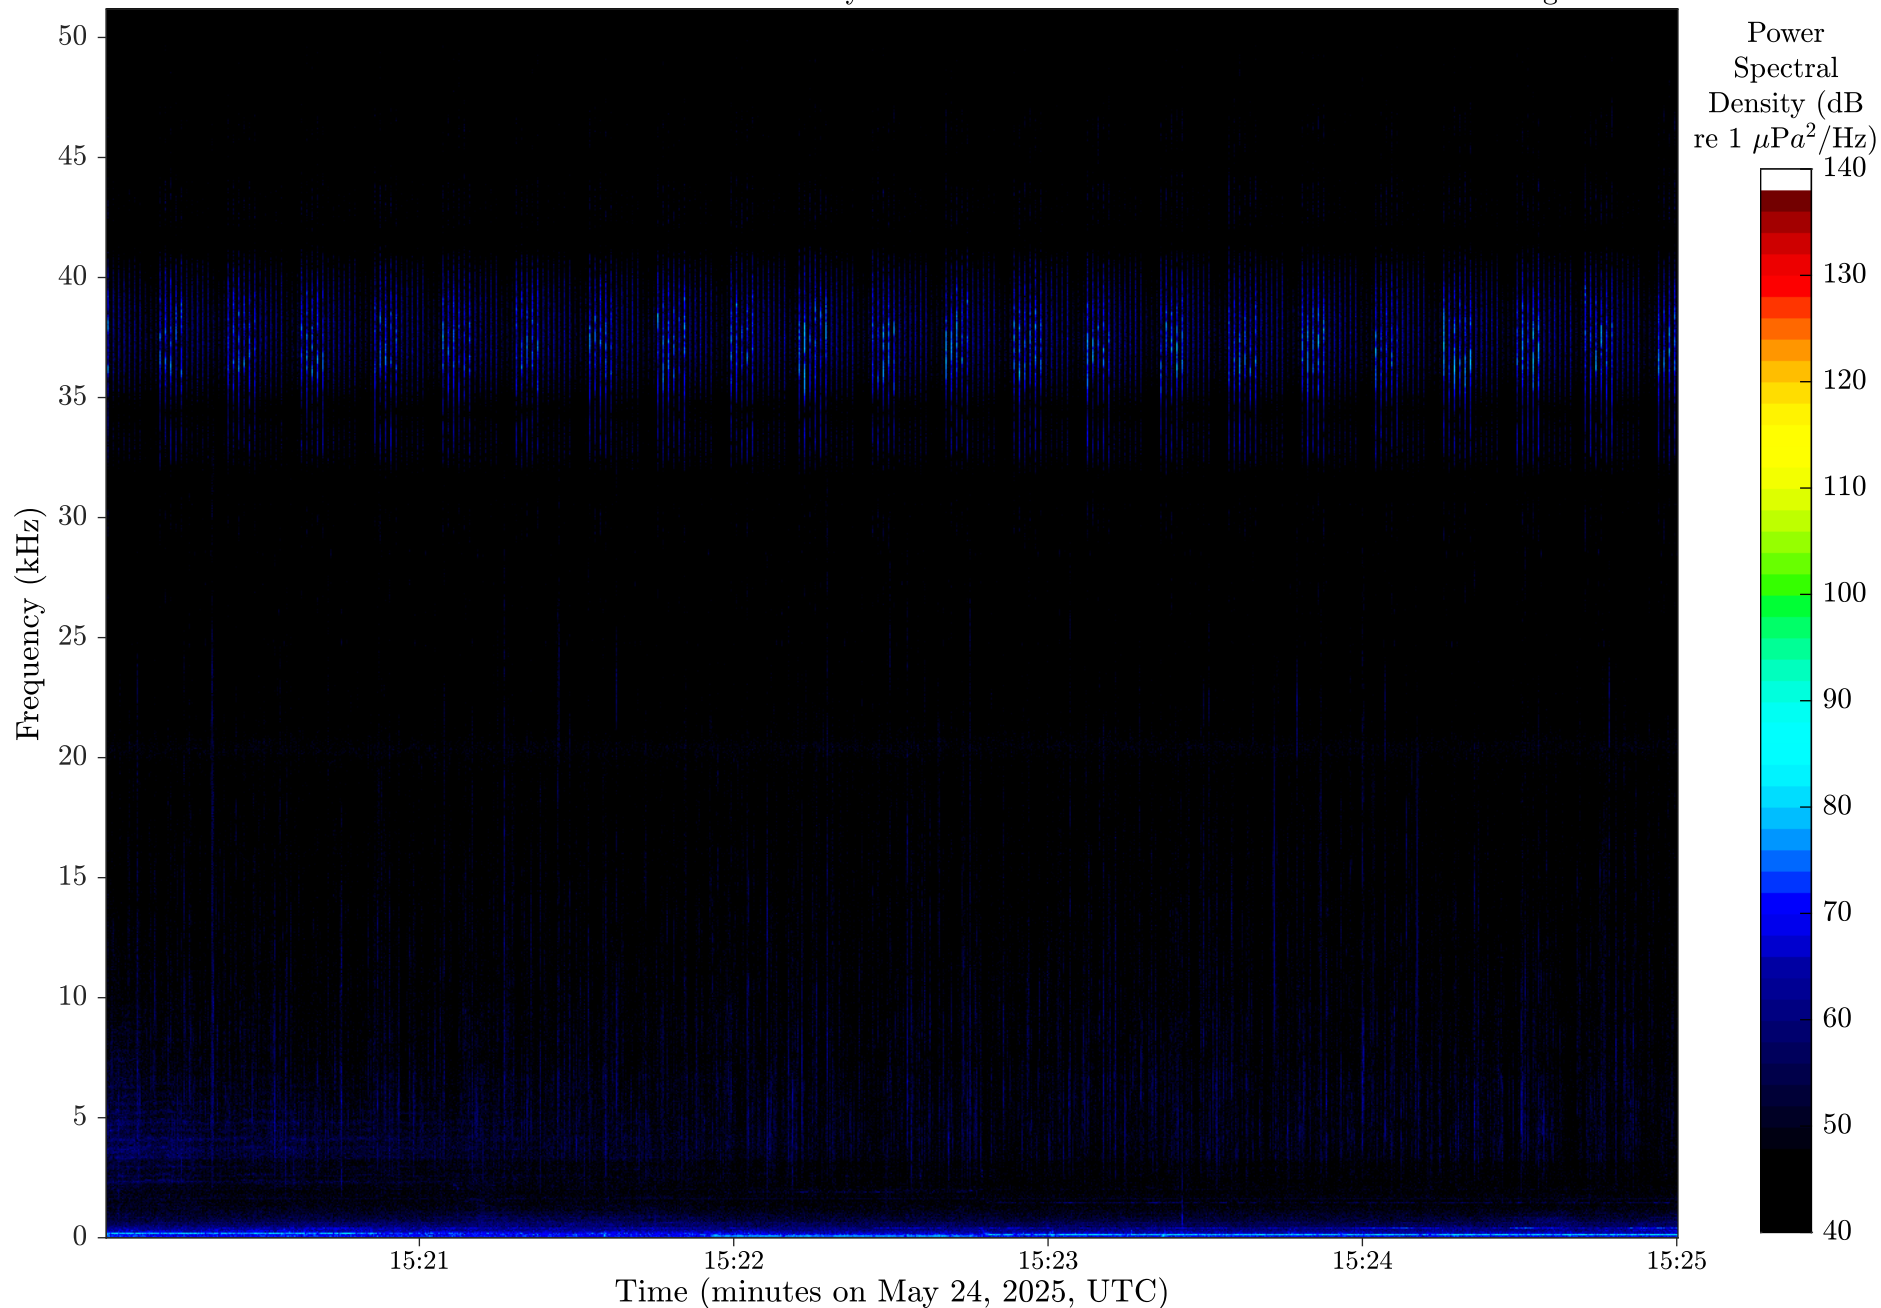


Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:38 UTC

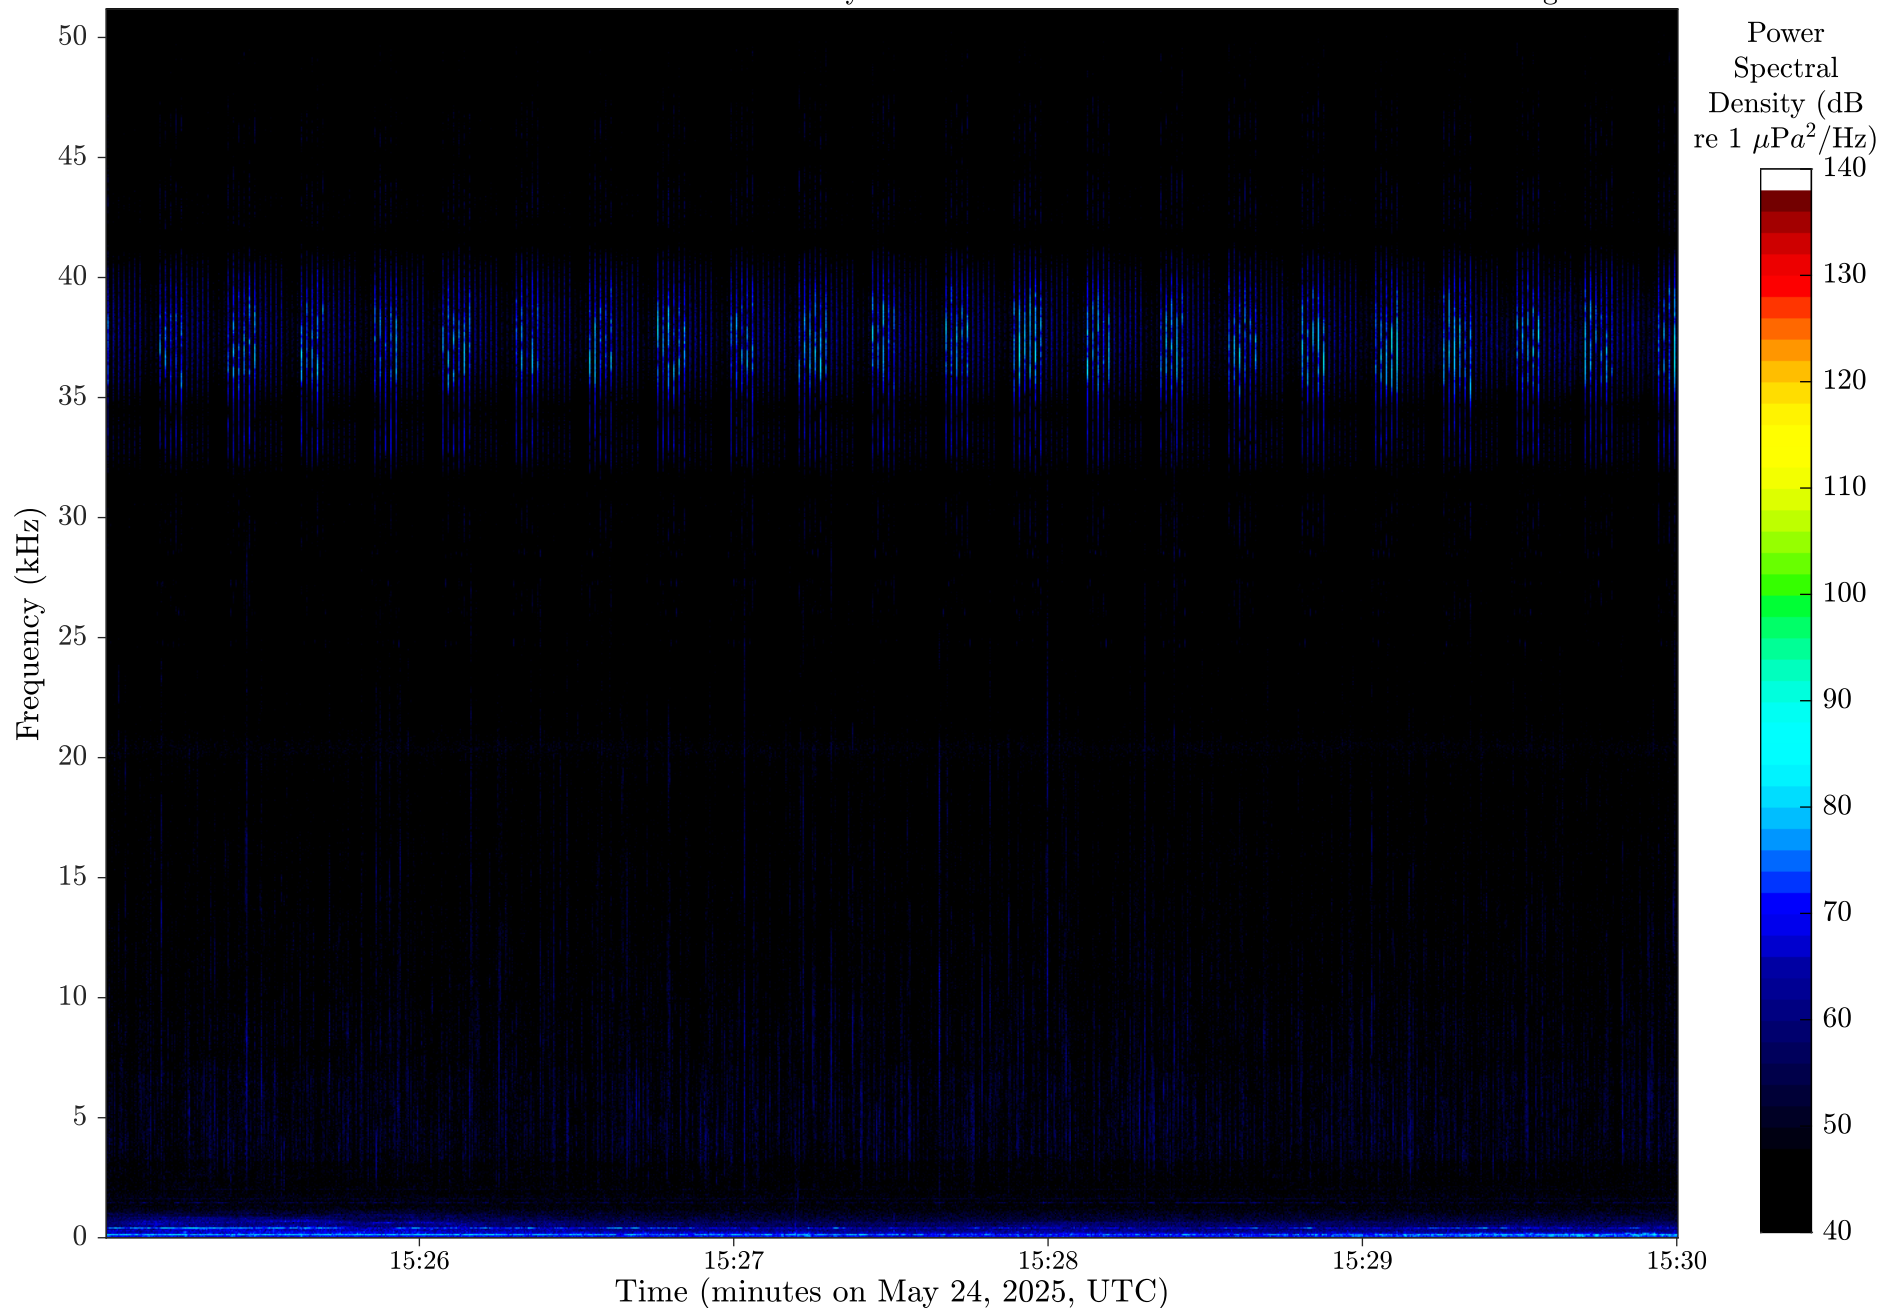


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:45 UTC

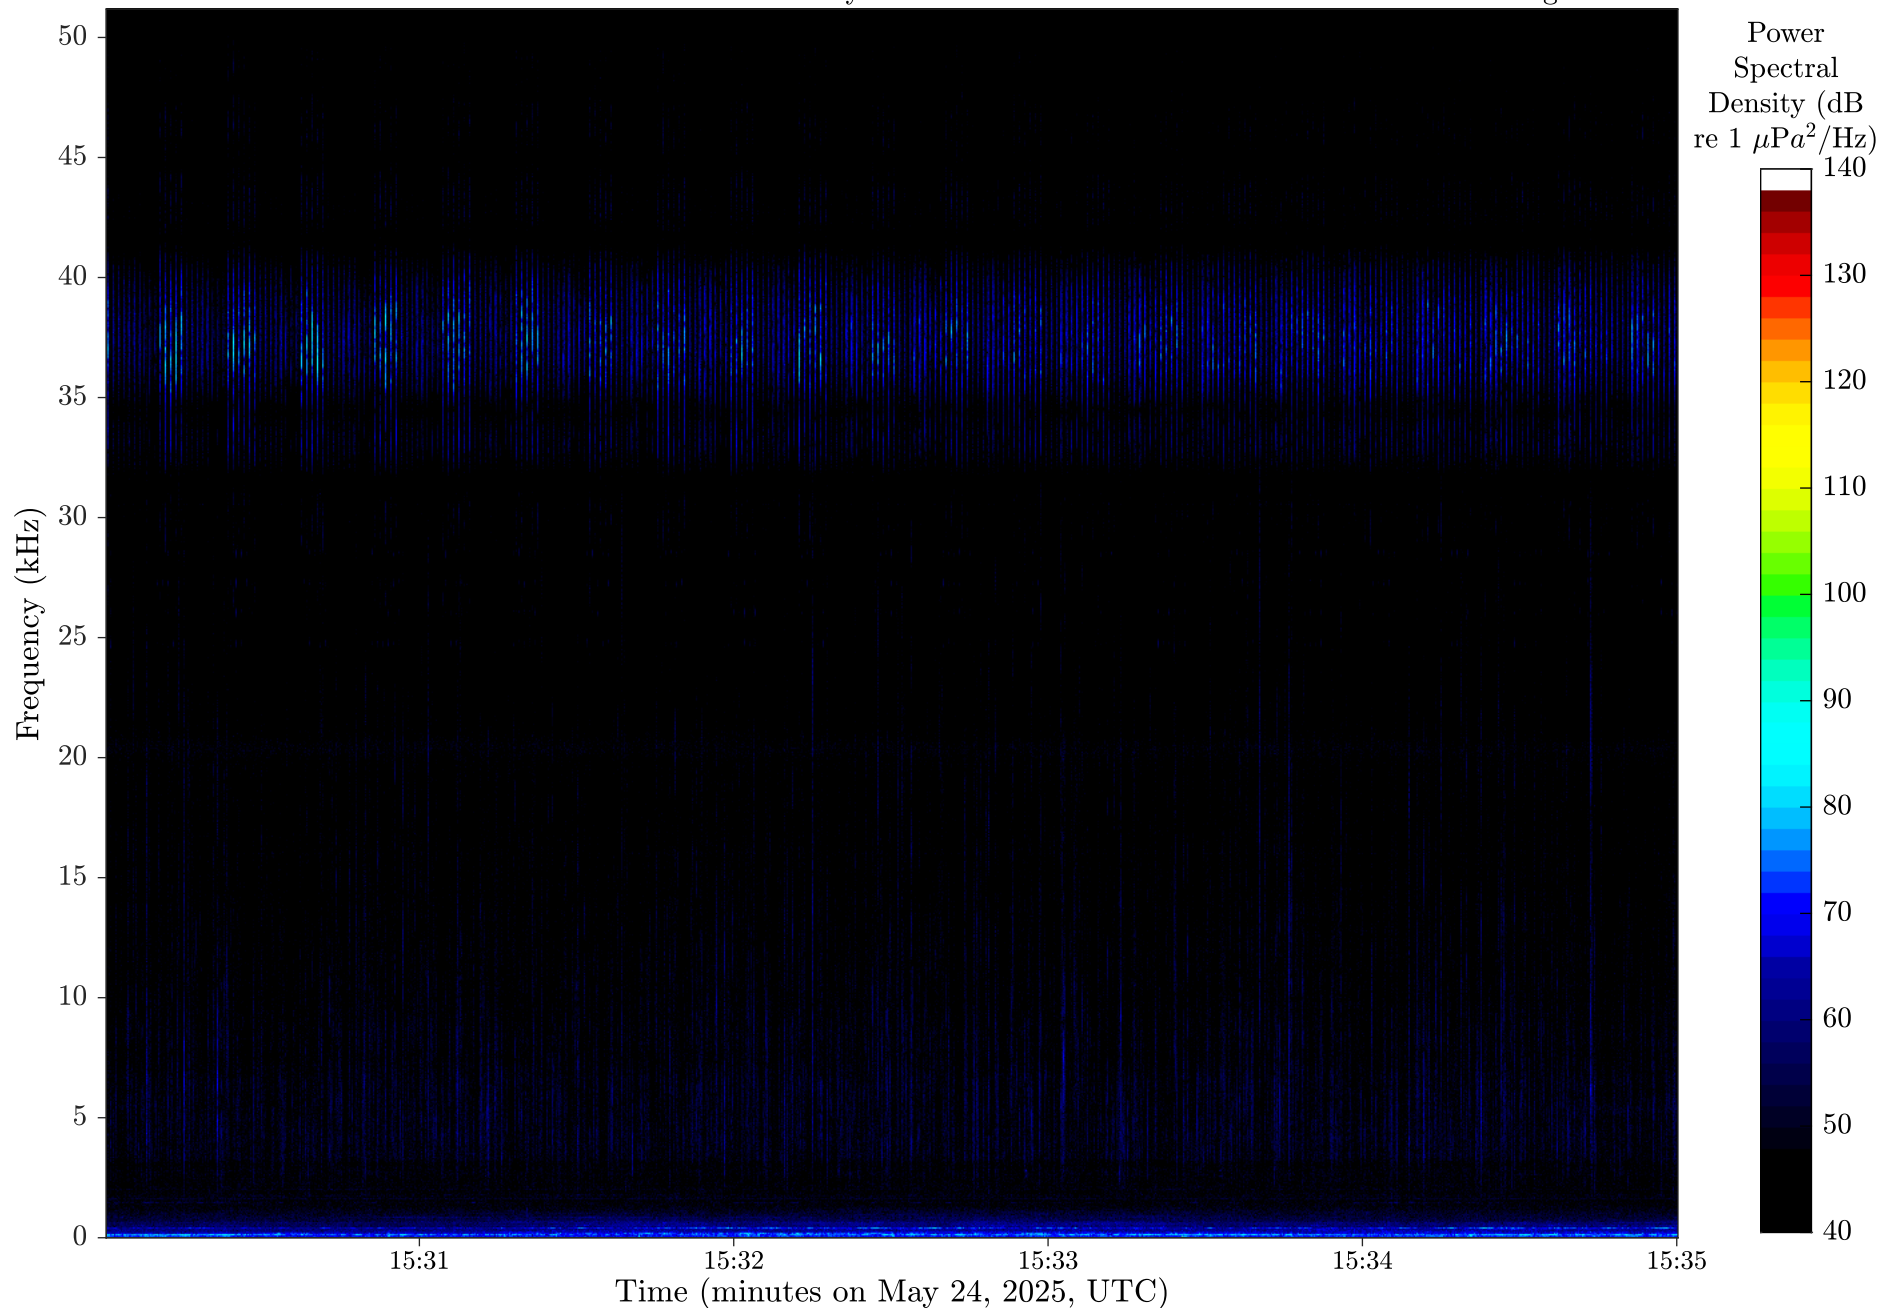


Comments: 32.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:52 UTC

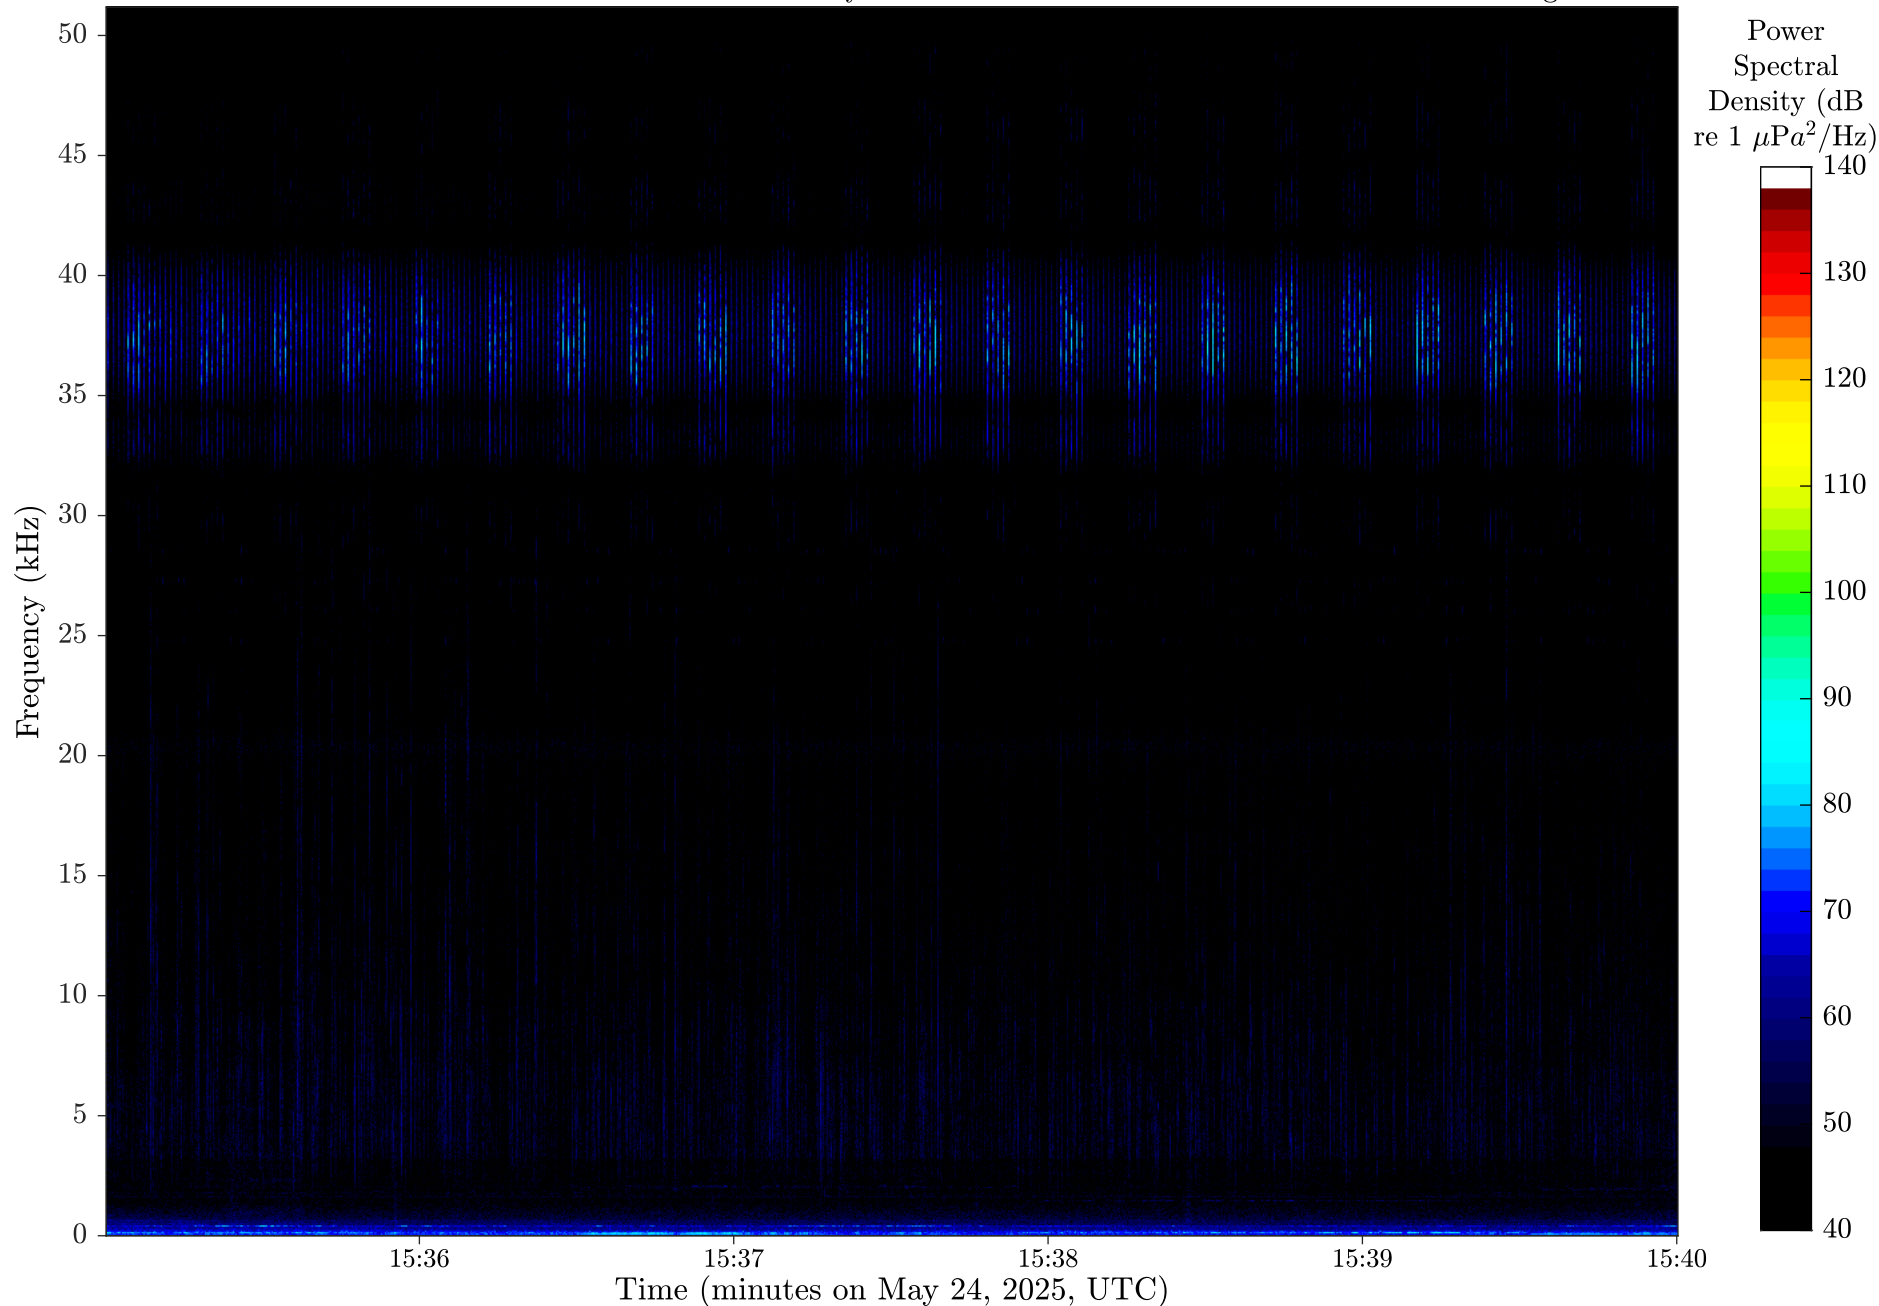


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:59 UTC

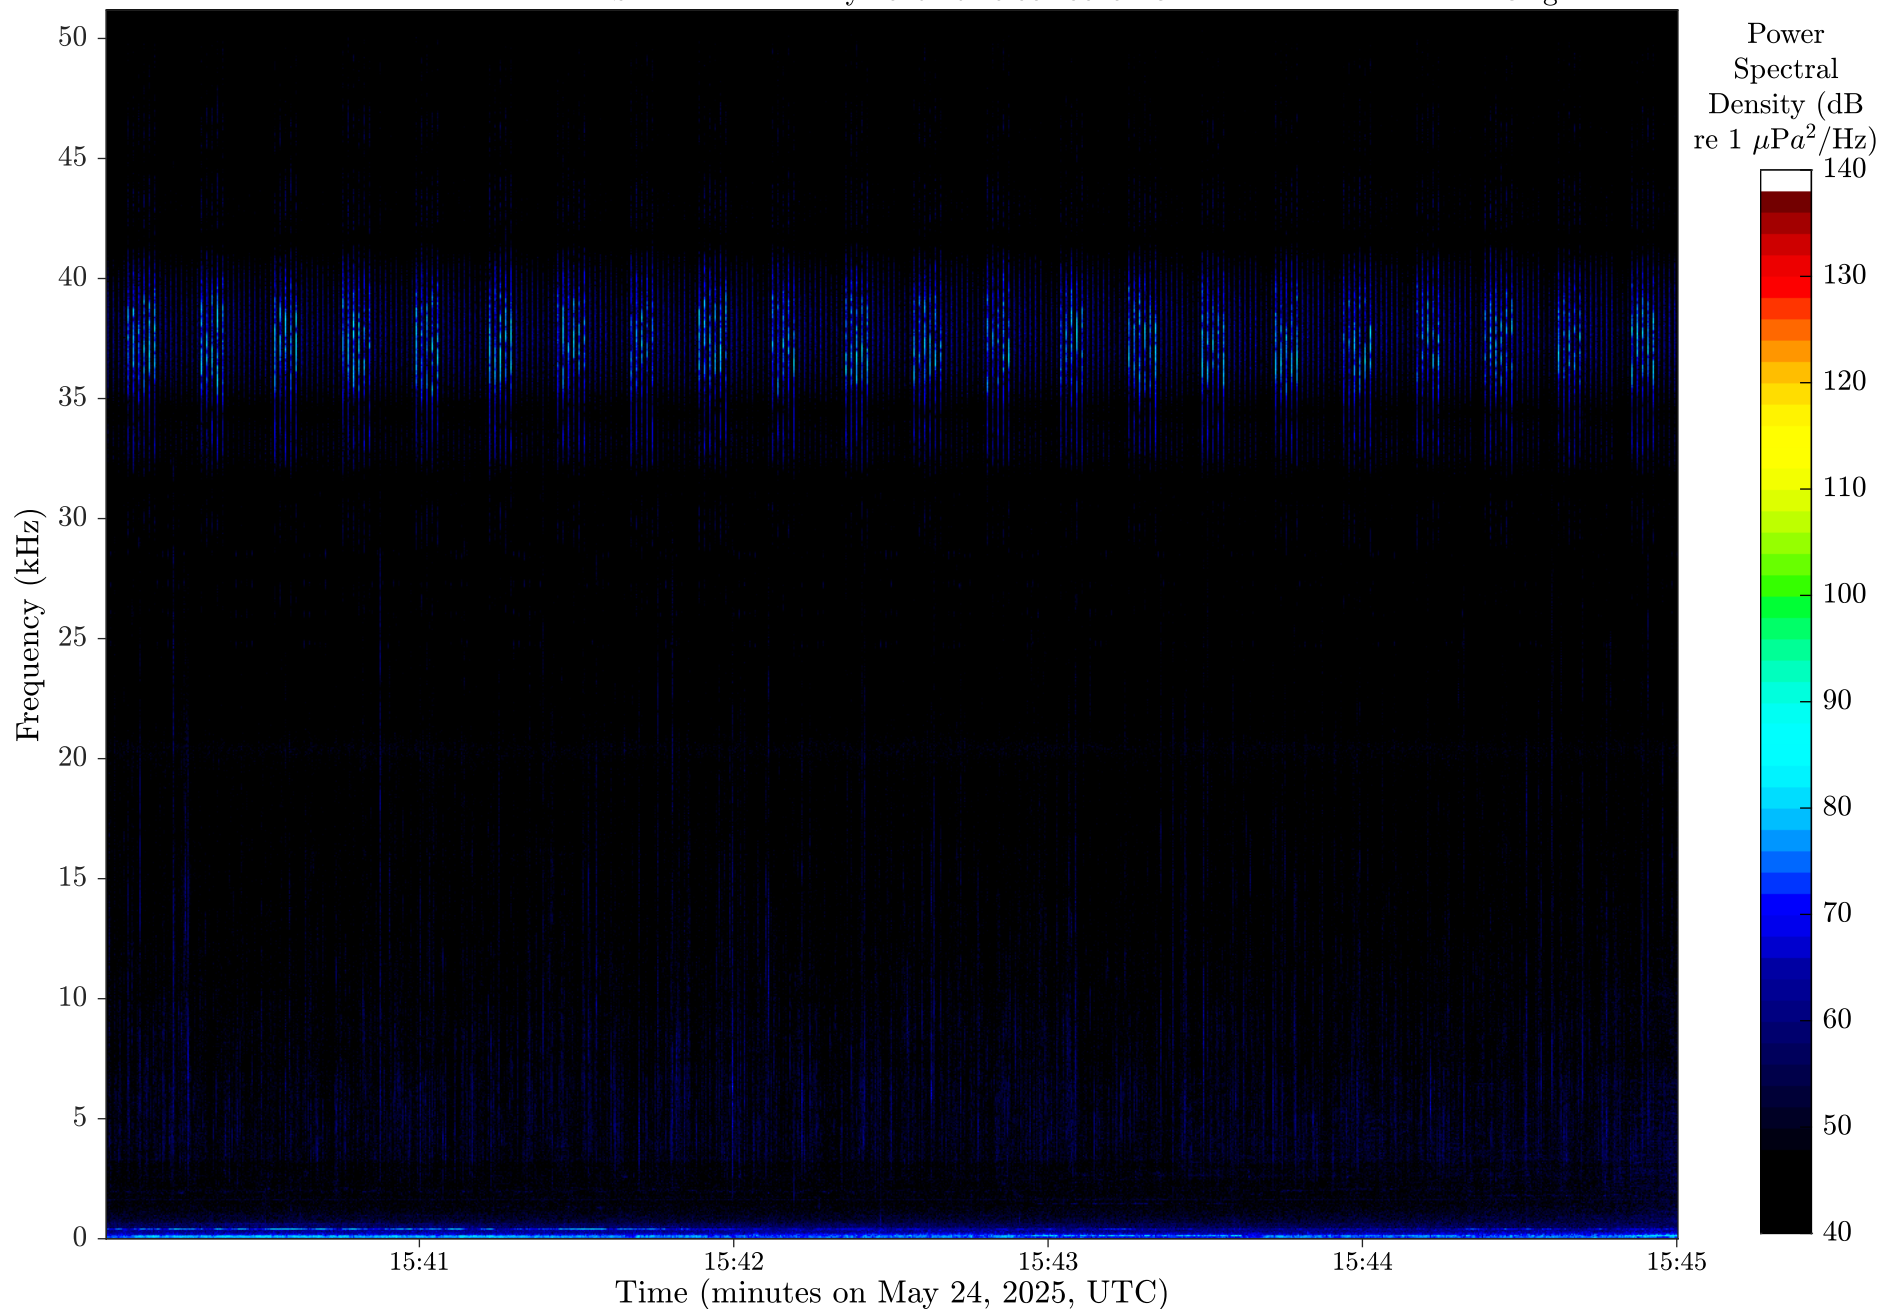


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:07 UTC

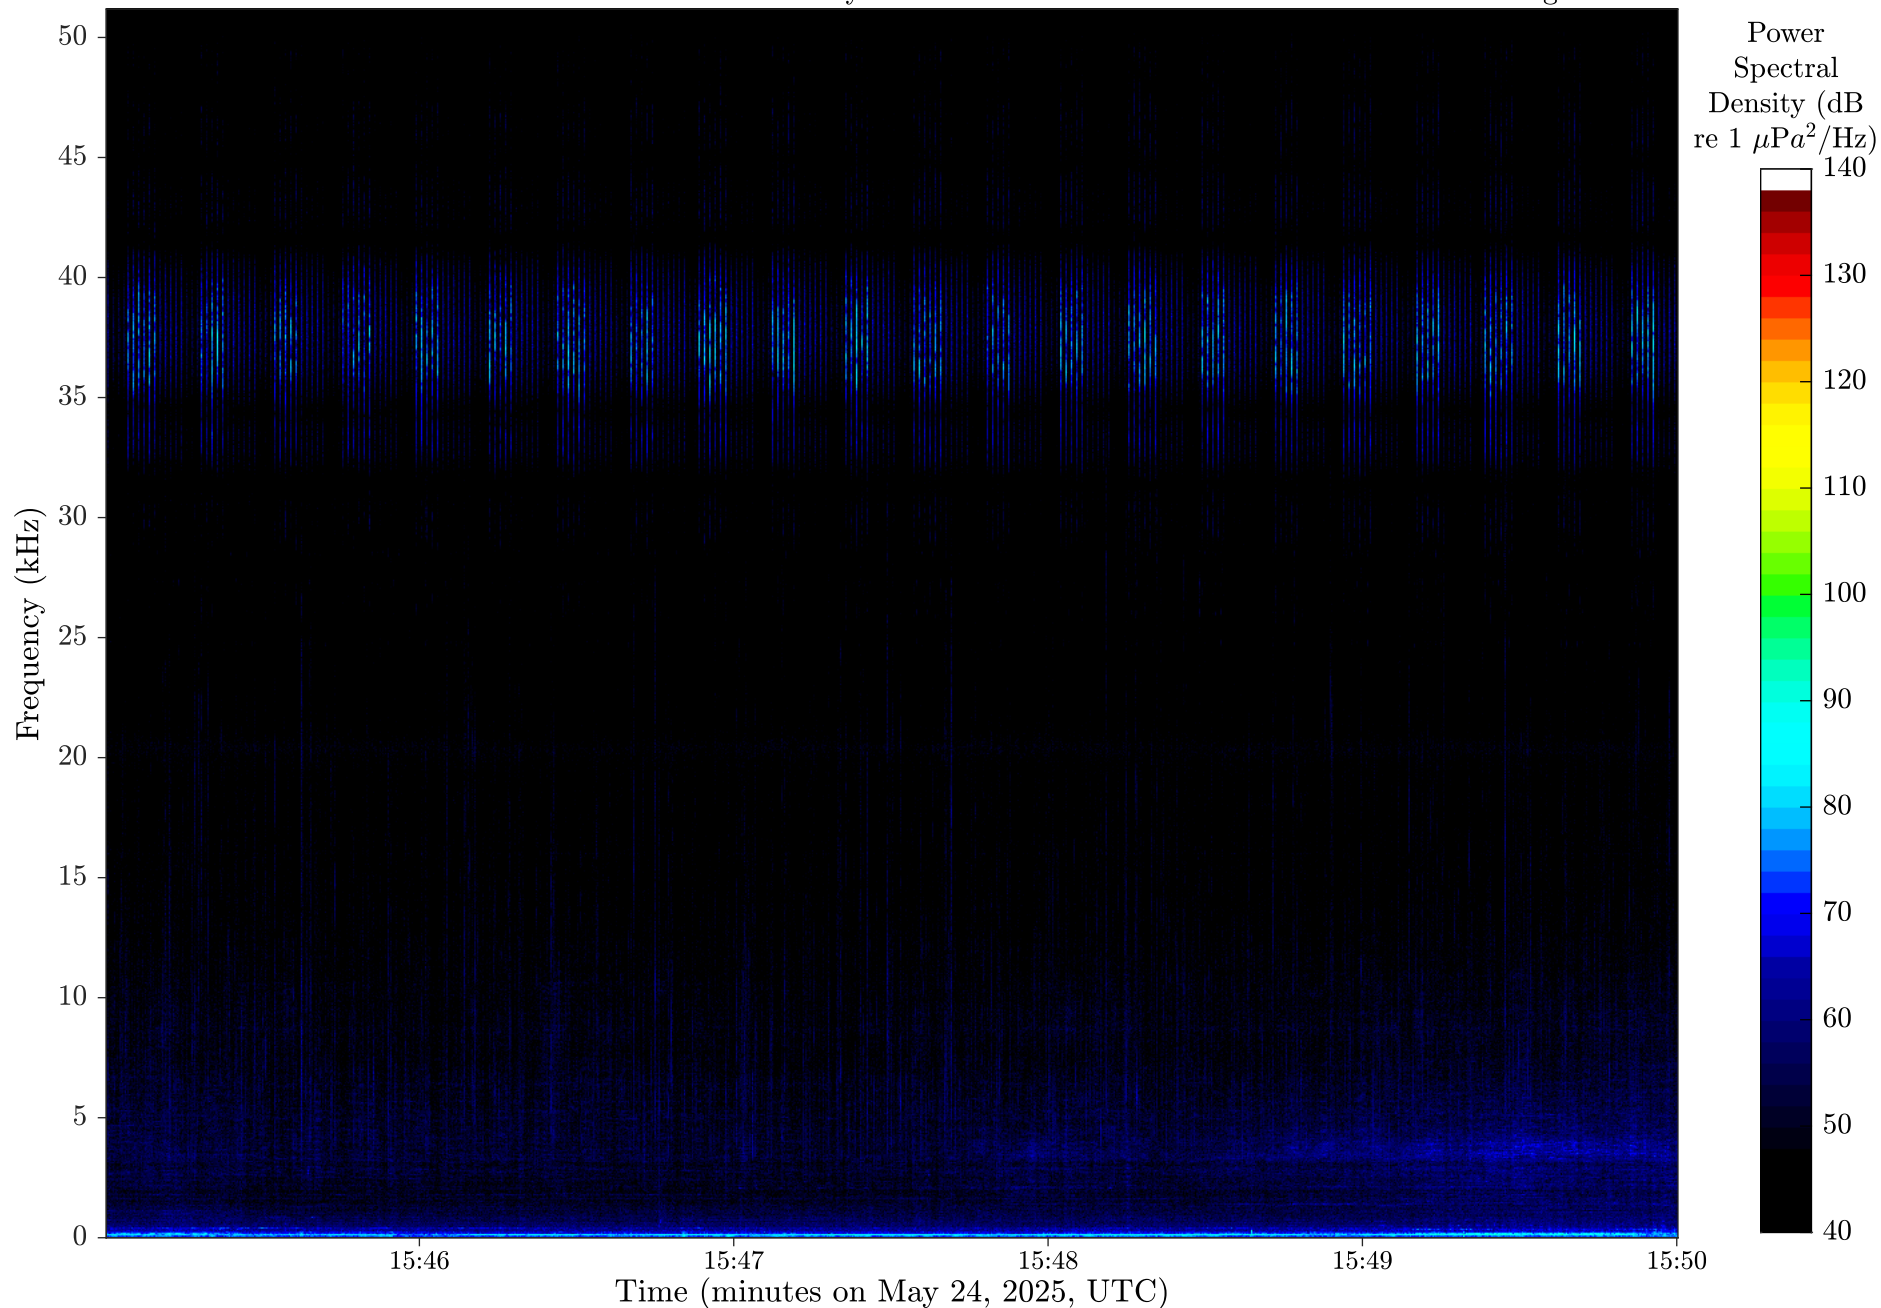


Comments: 32.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:35:14 UTC

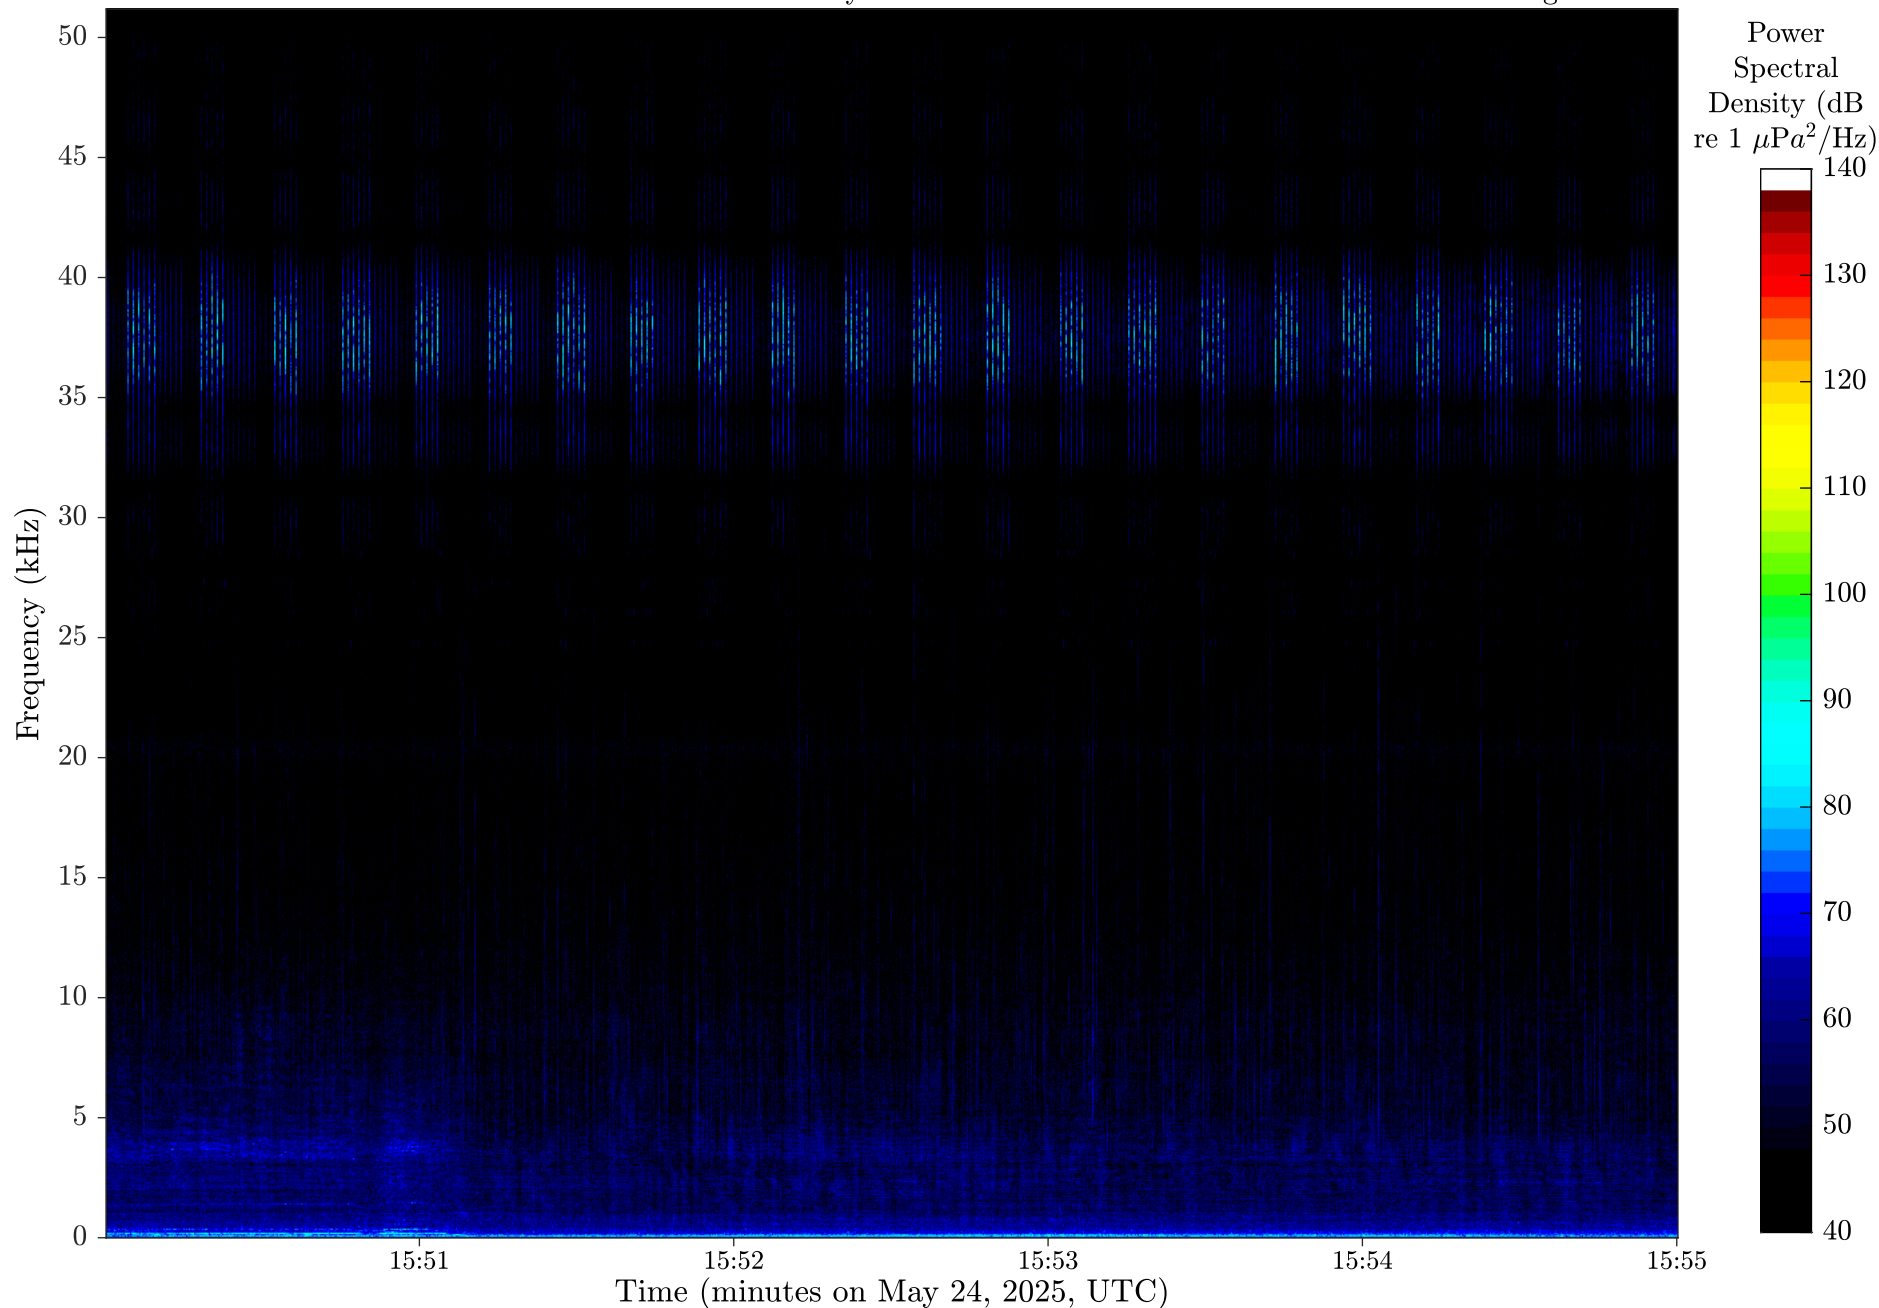

Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:35:21 UTC

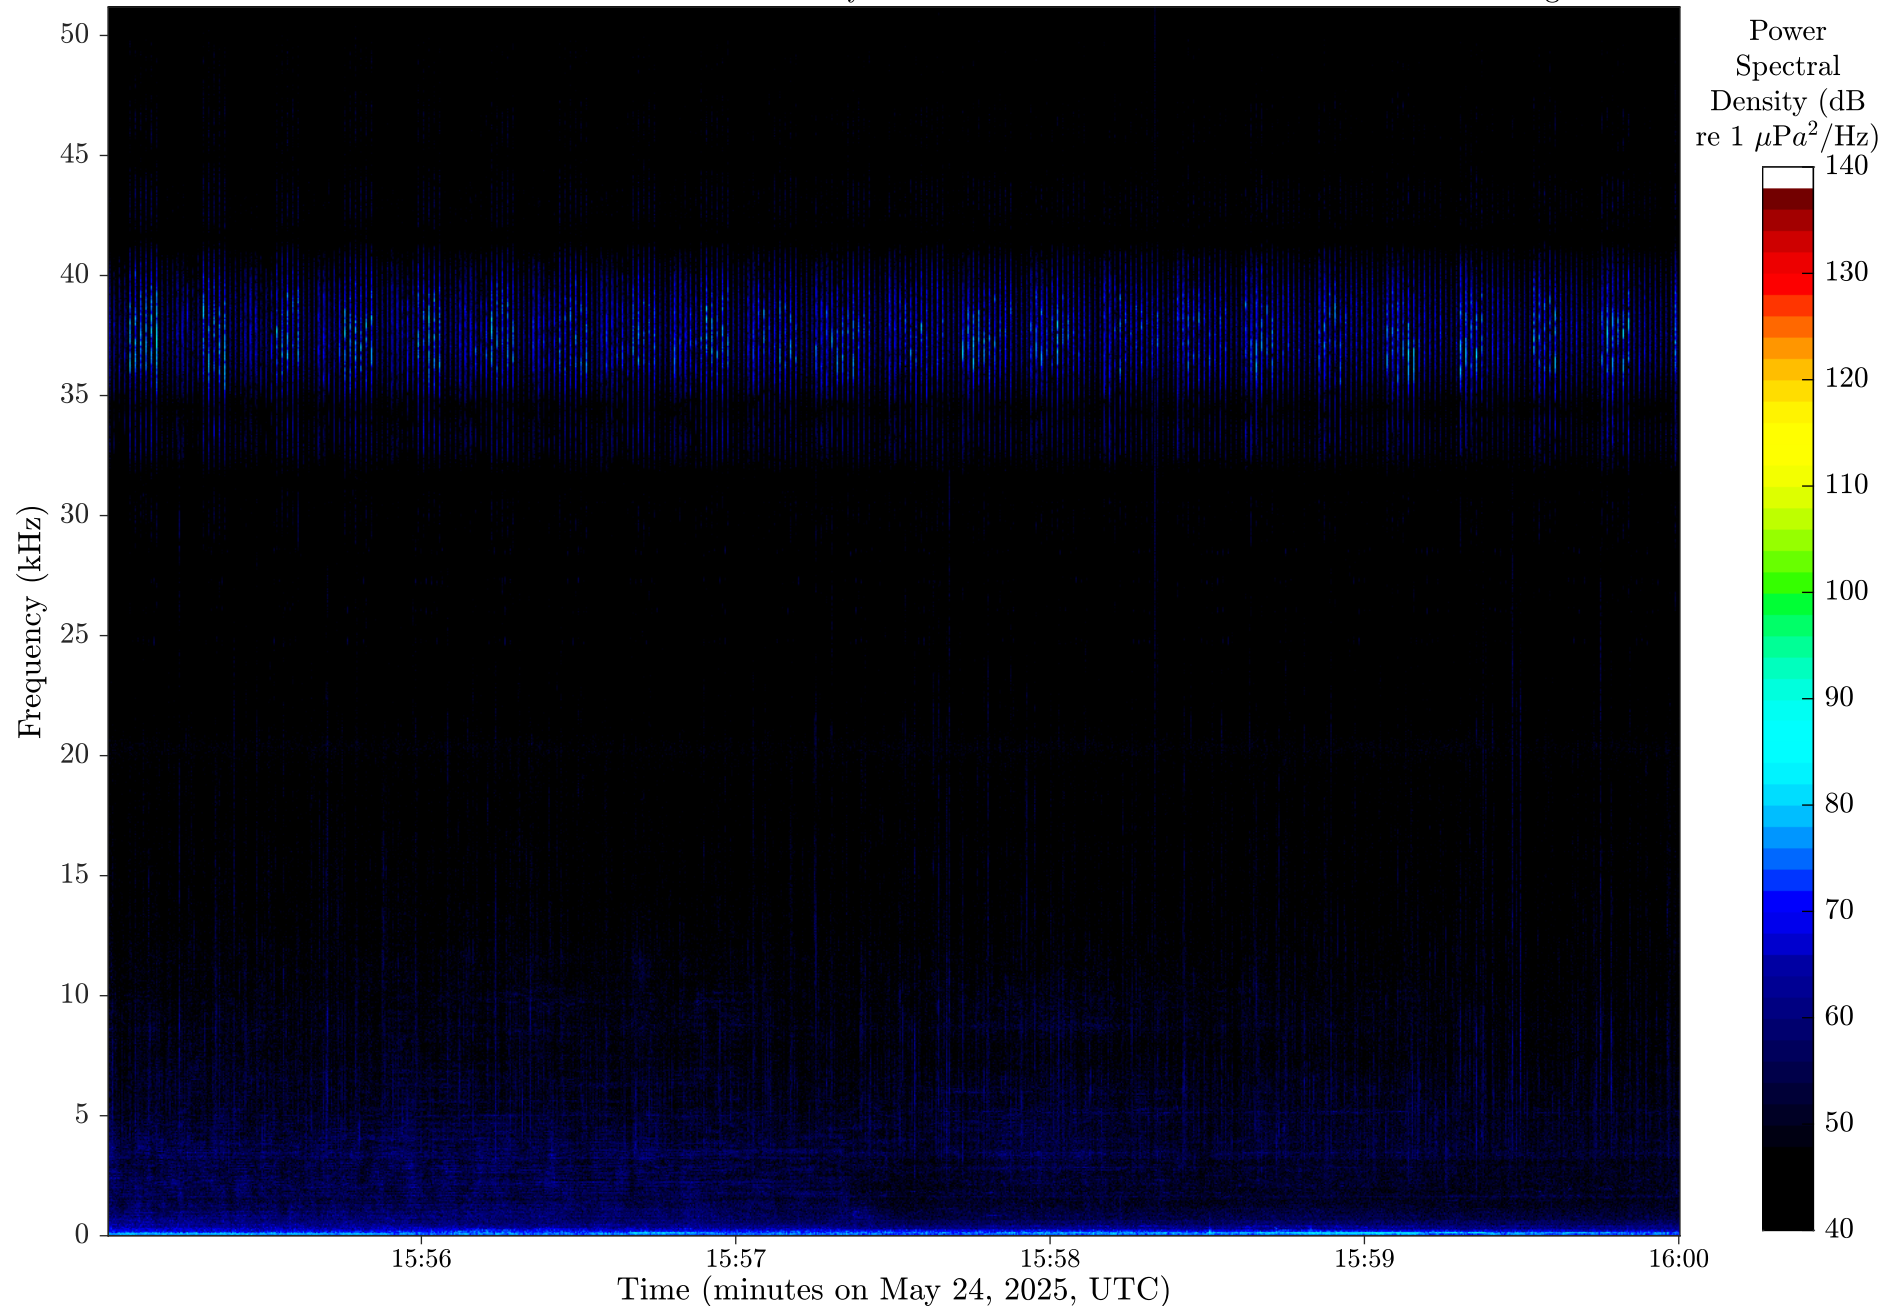

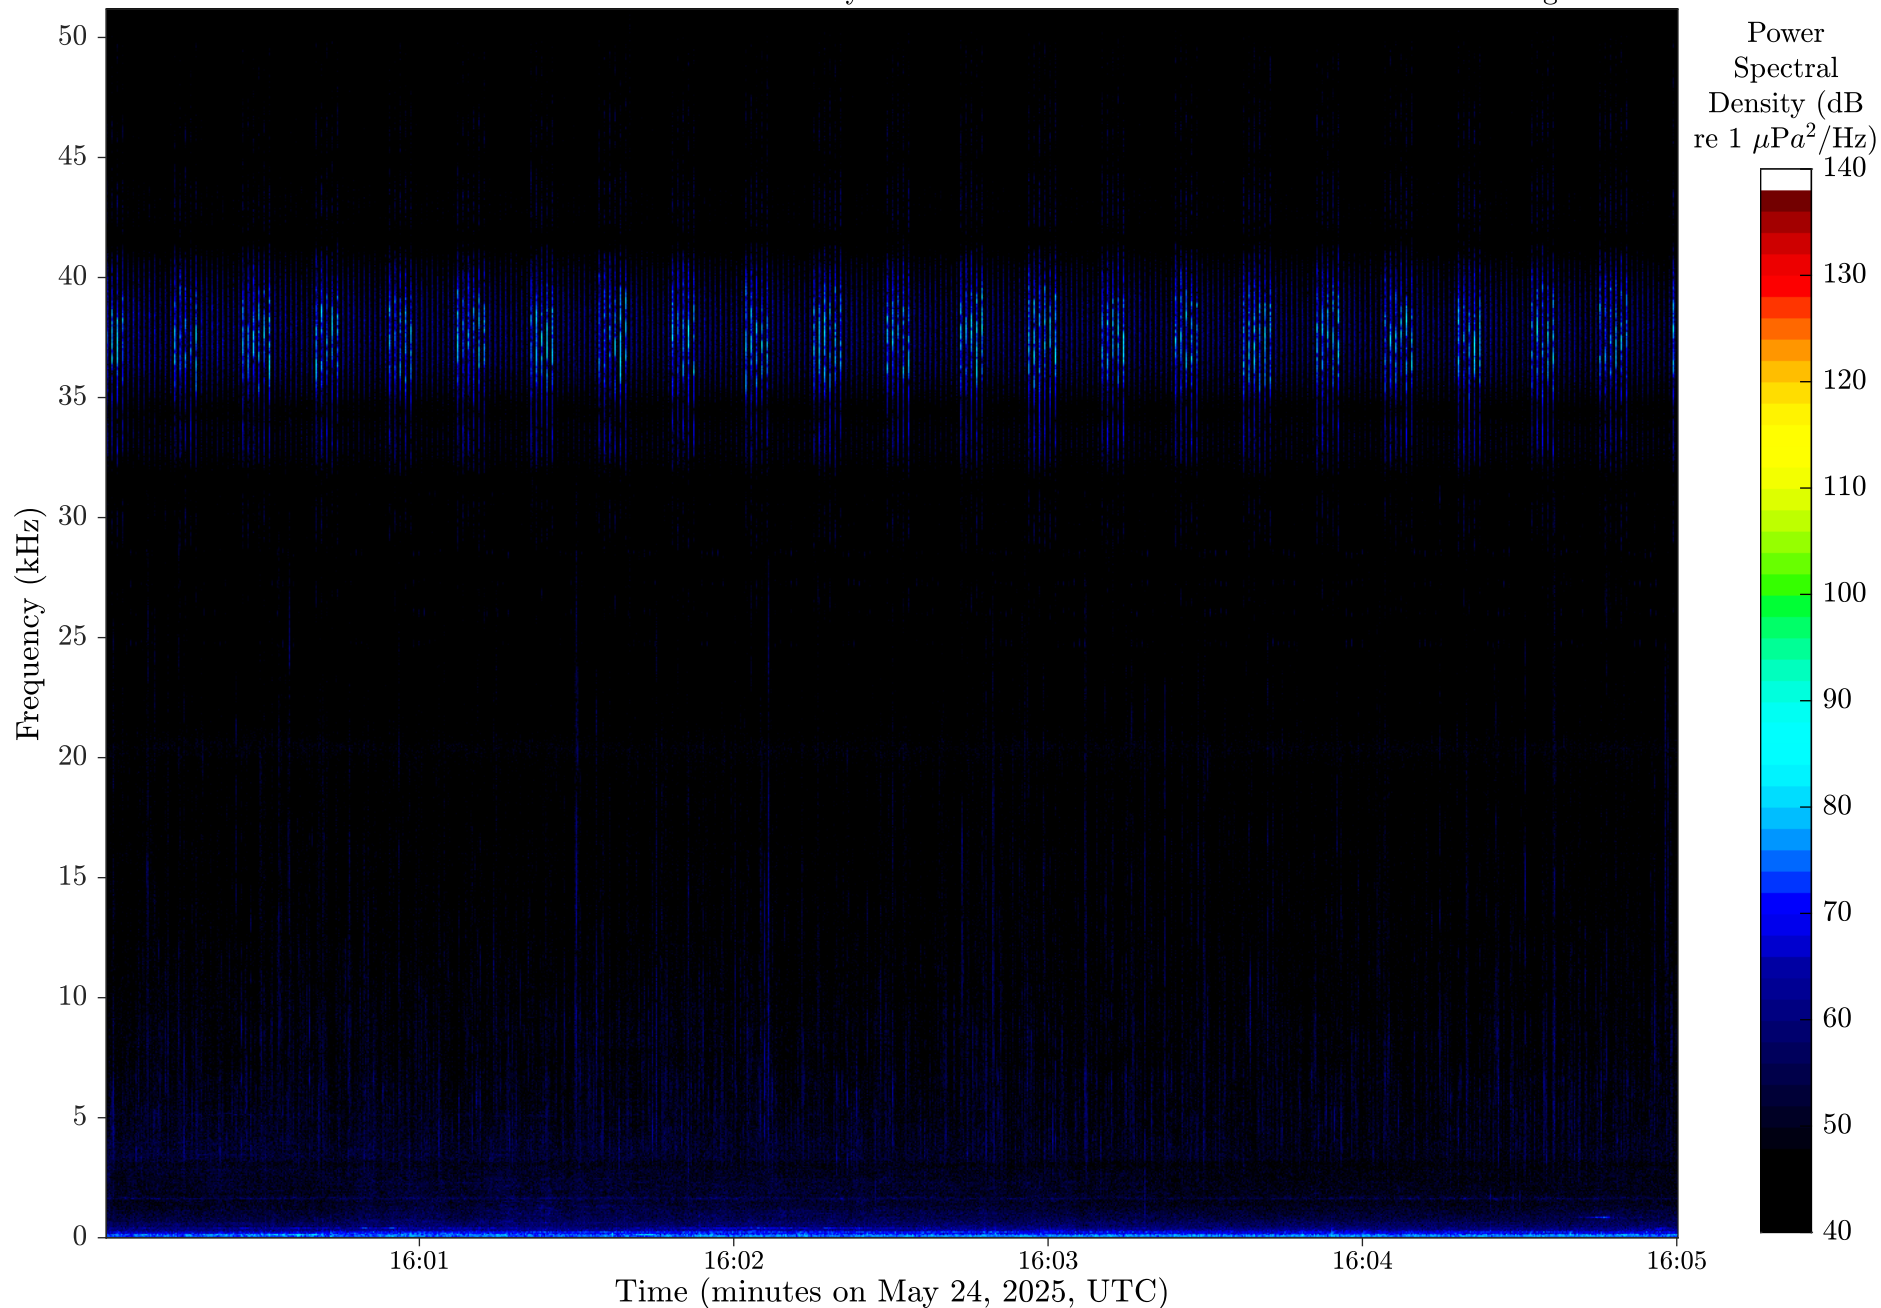


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:35 UTC

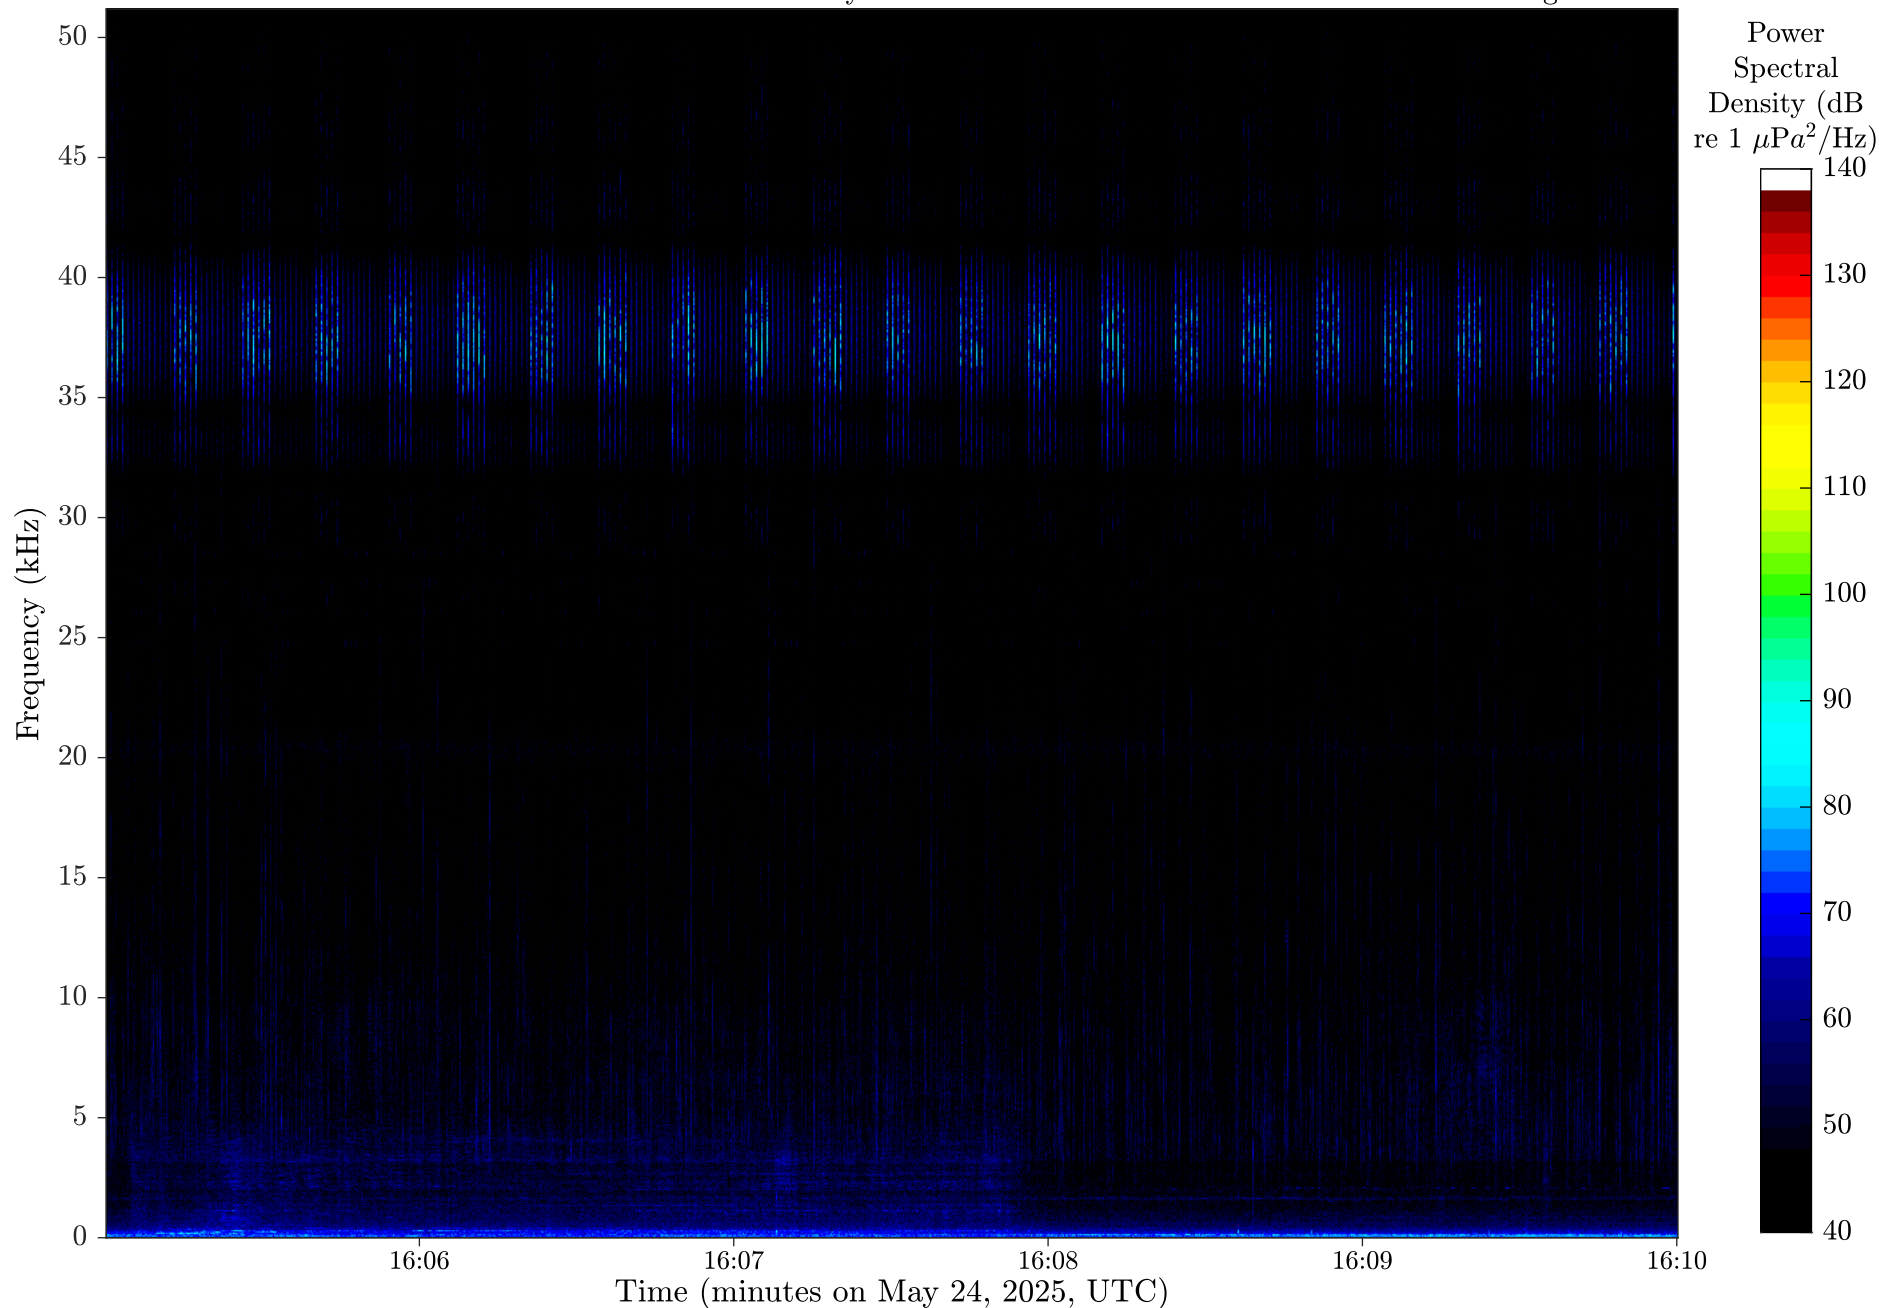


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:35:42 UTC

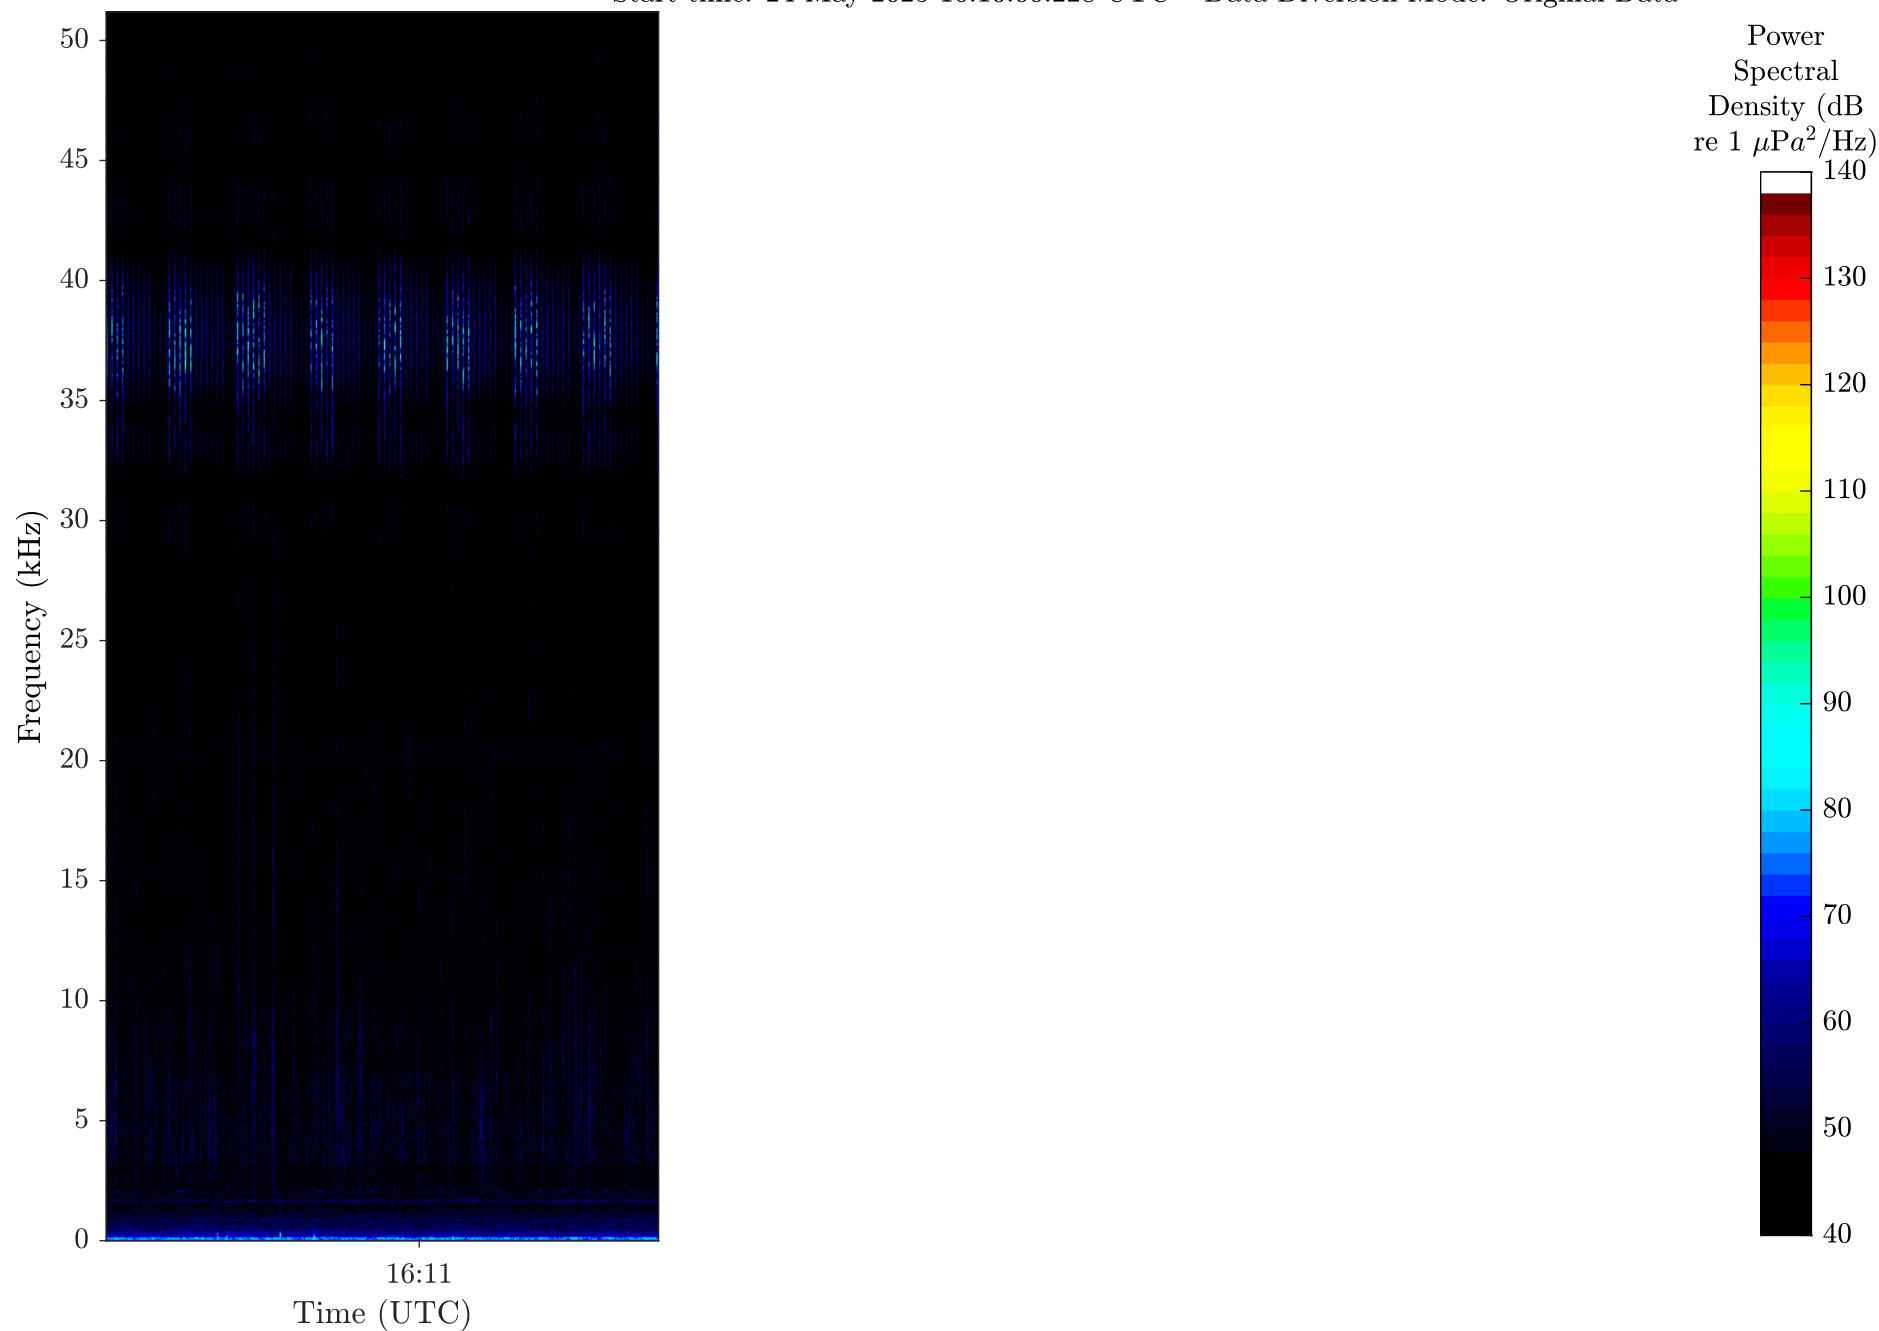

Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:35:46 UTC

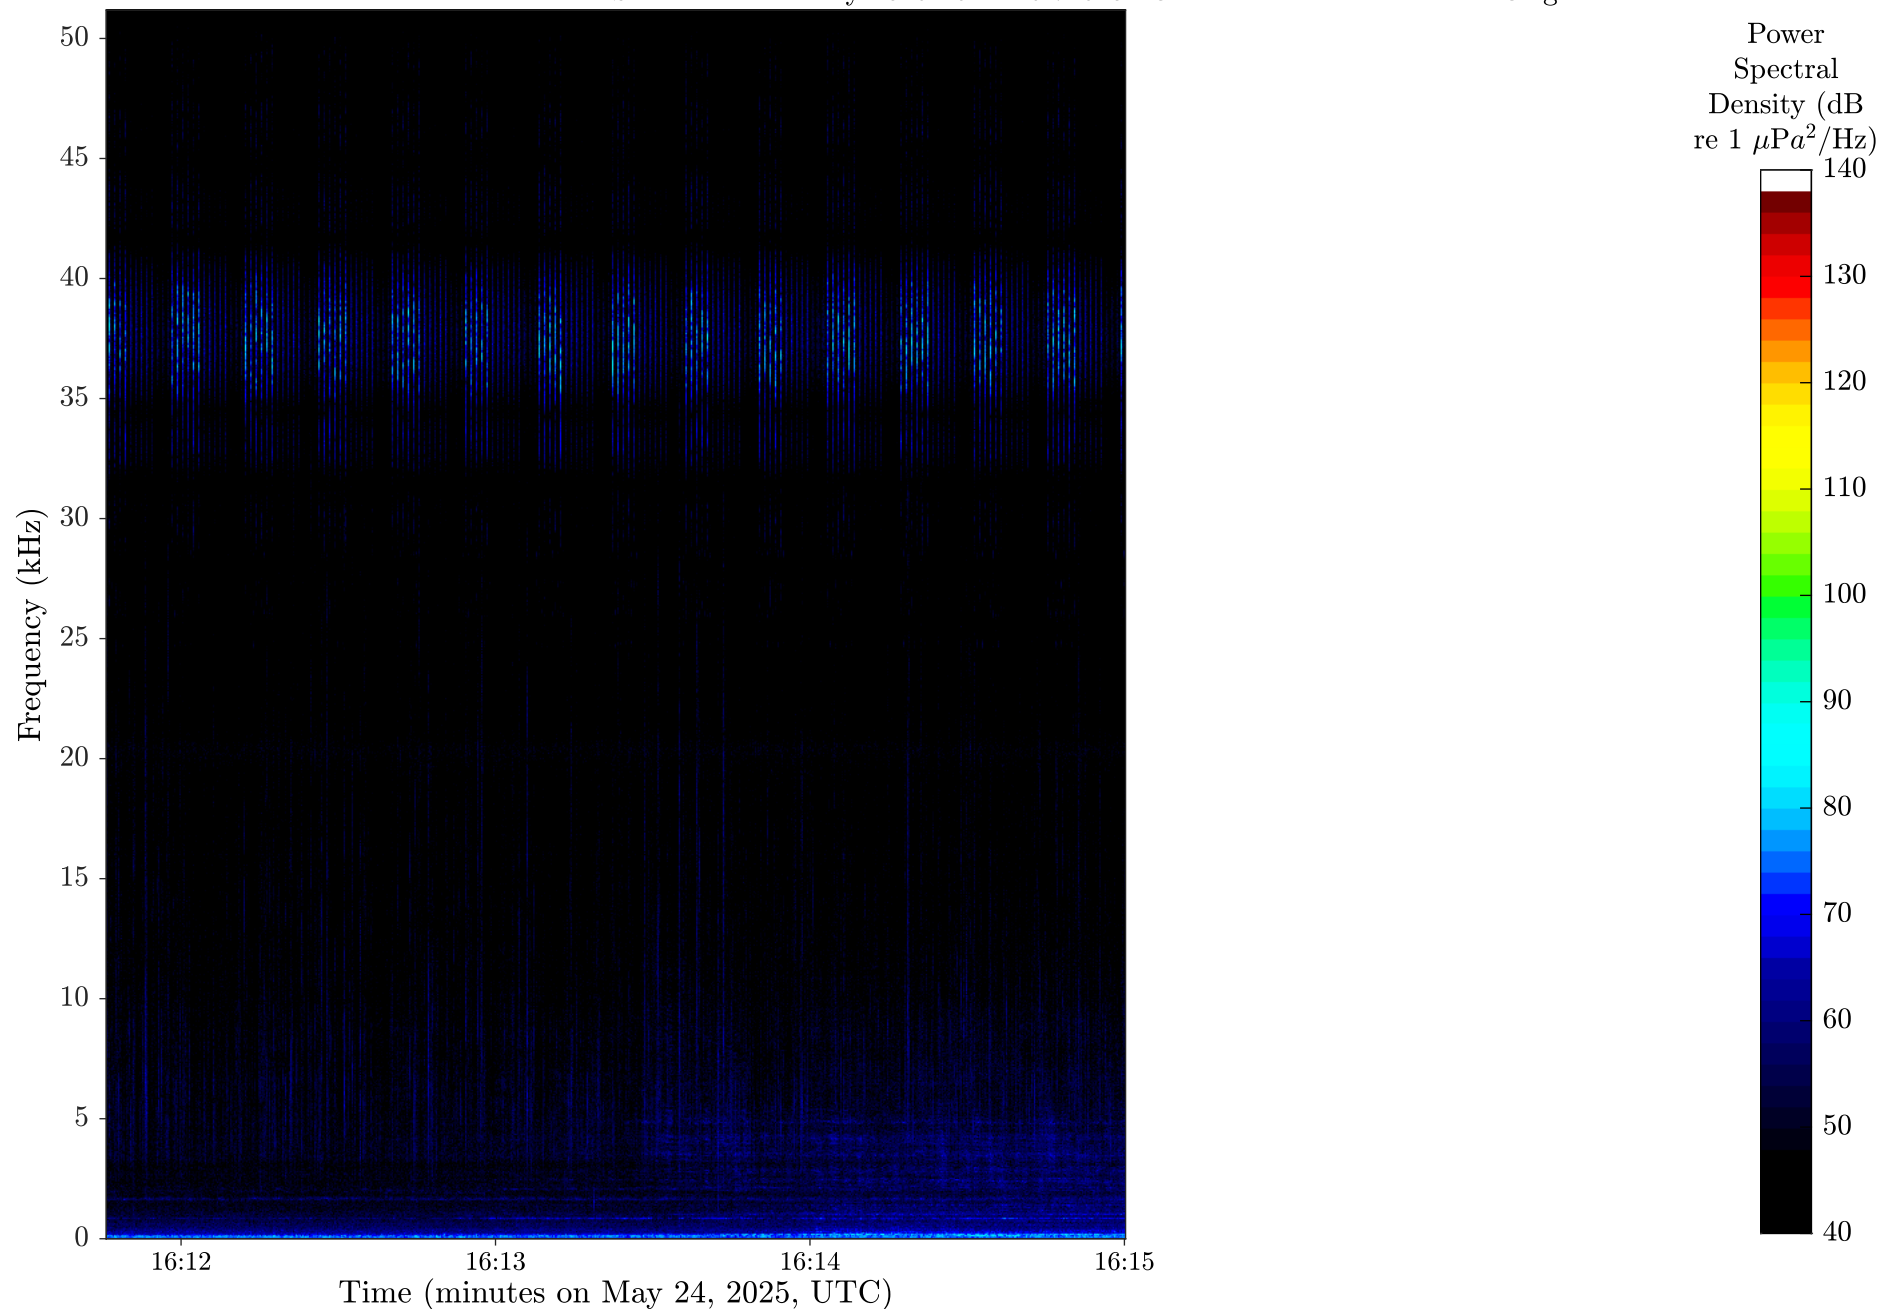

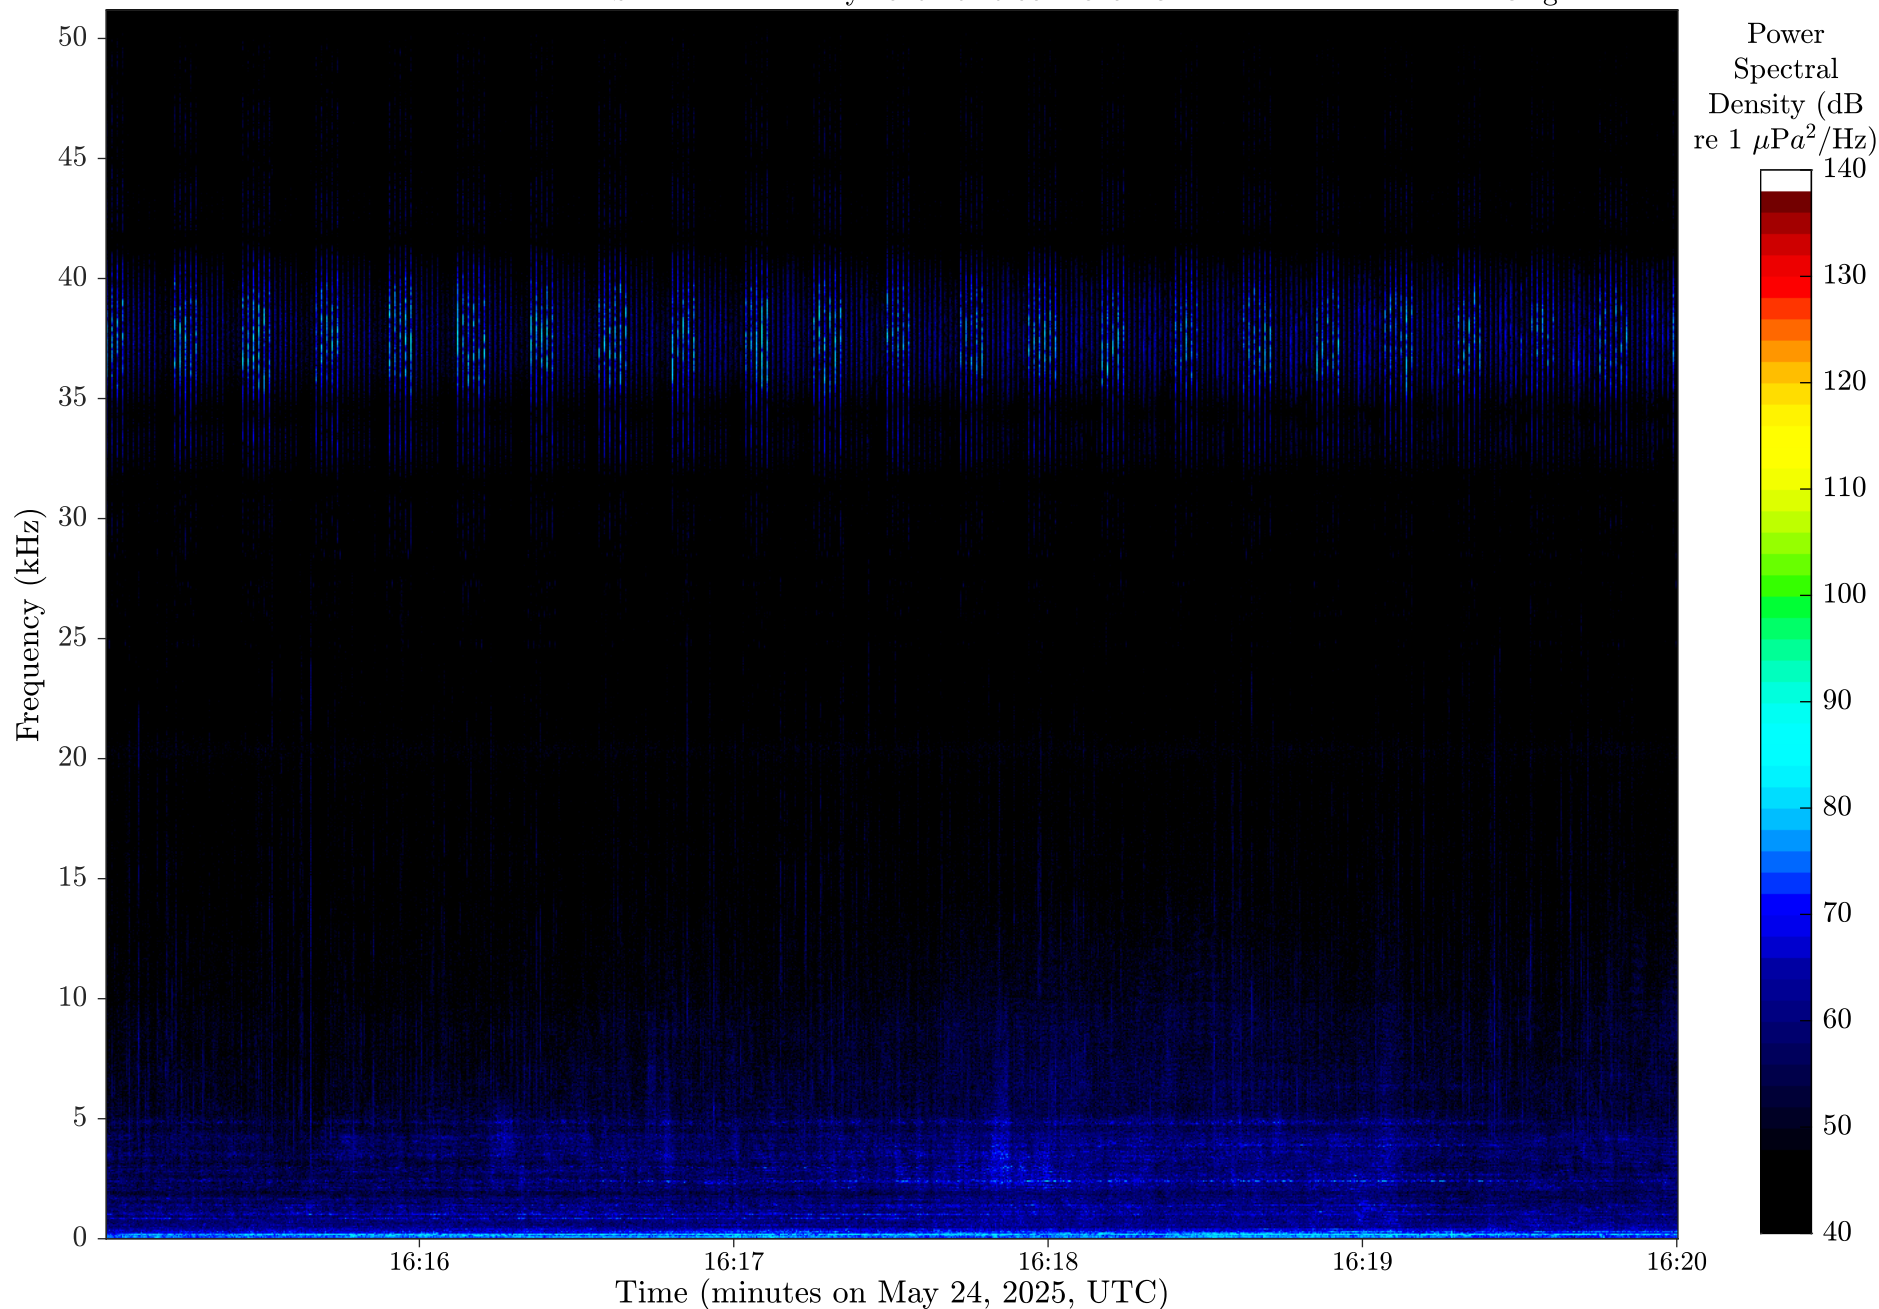


Comments: 29.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:58 UTC

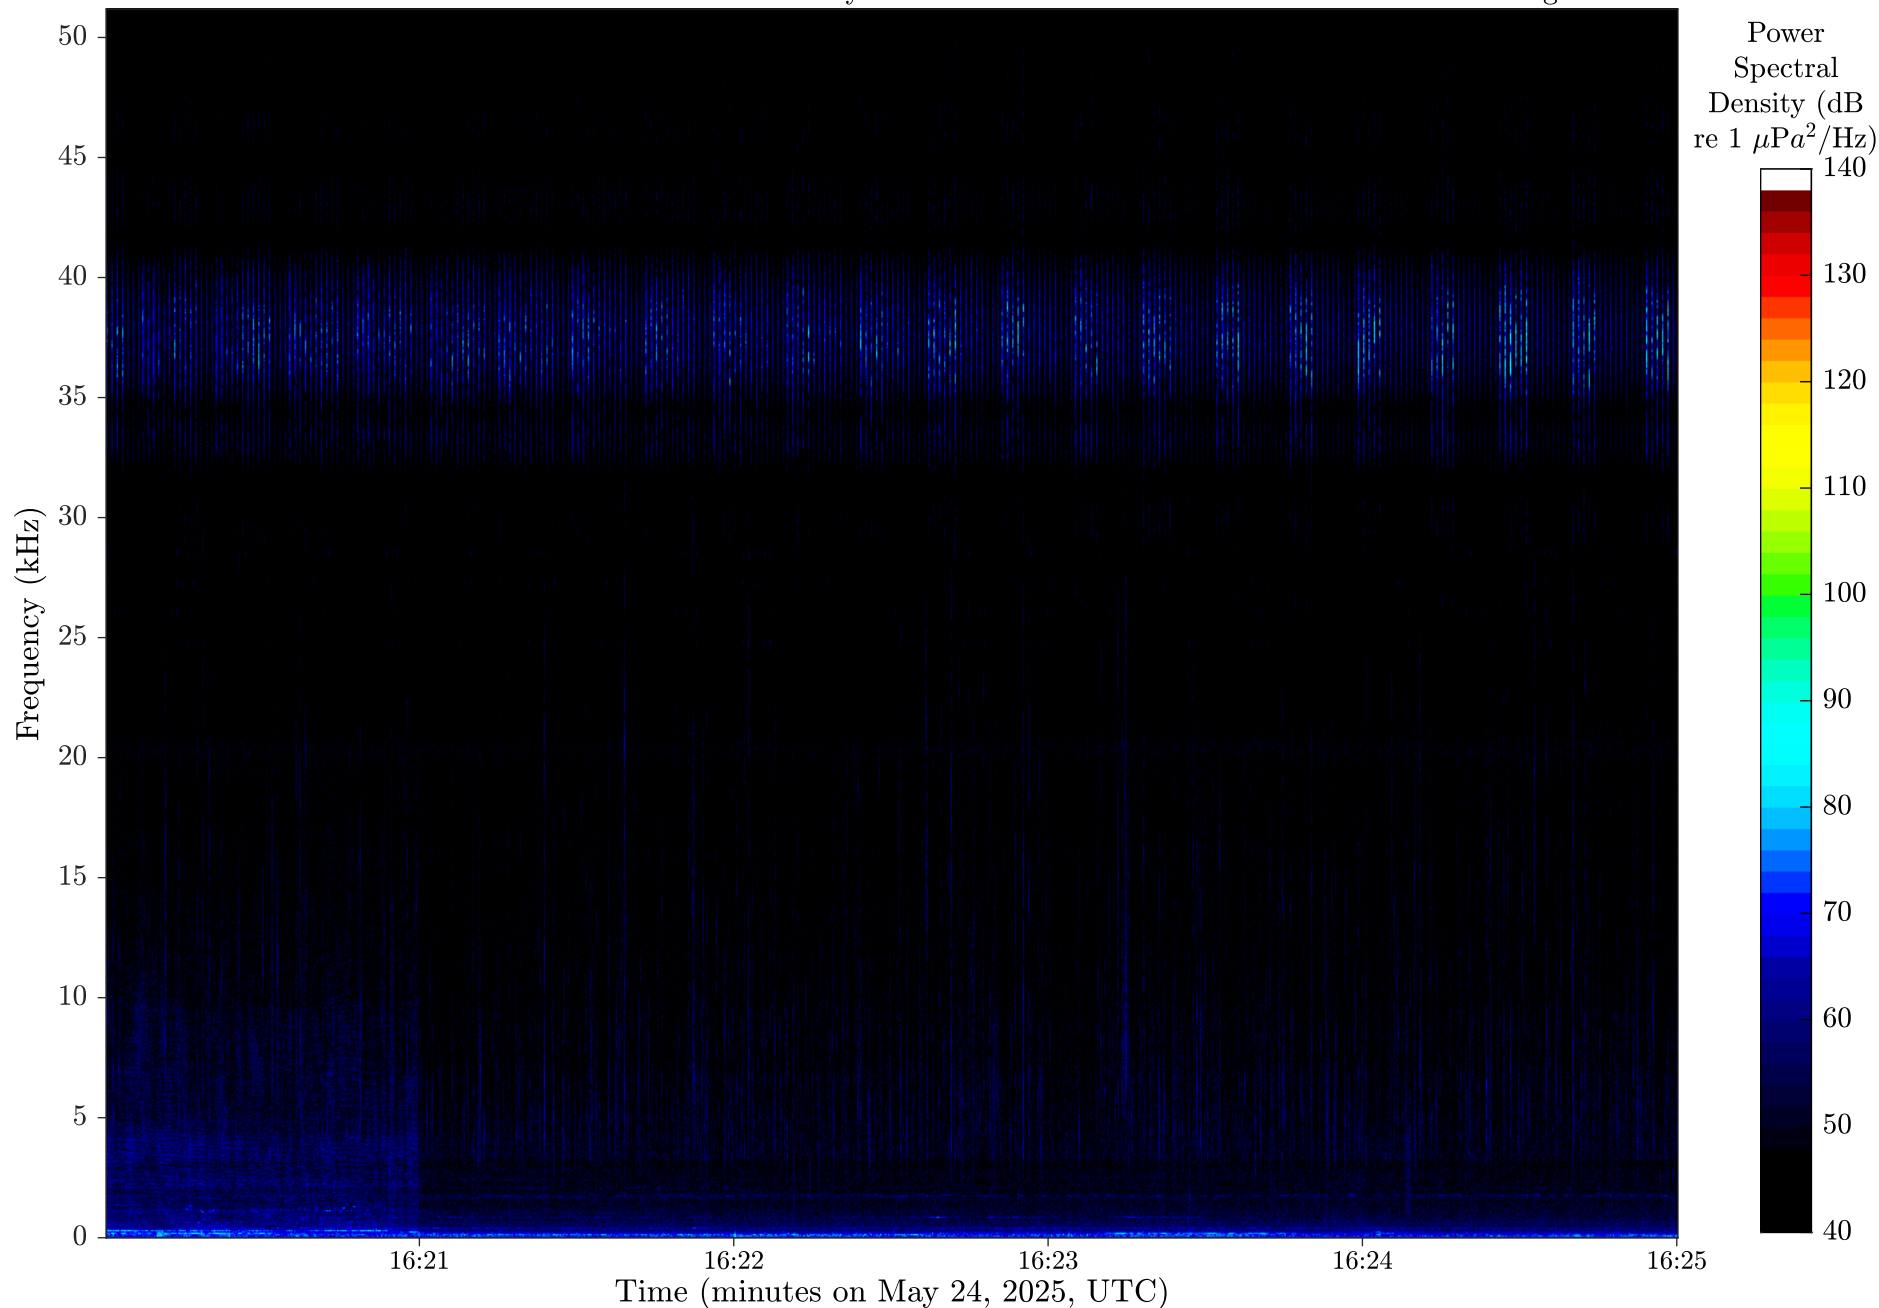


Comments: 29.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:05 UTC

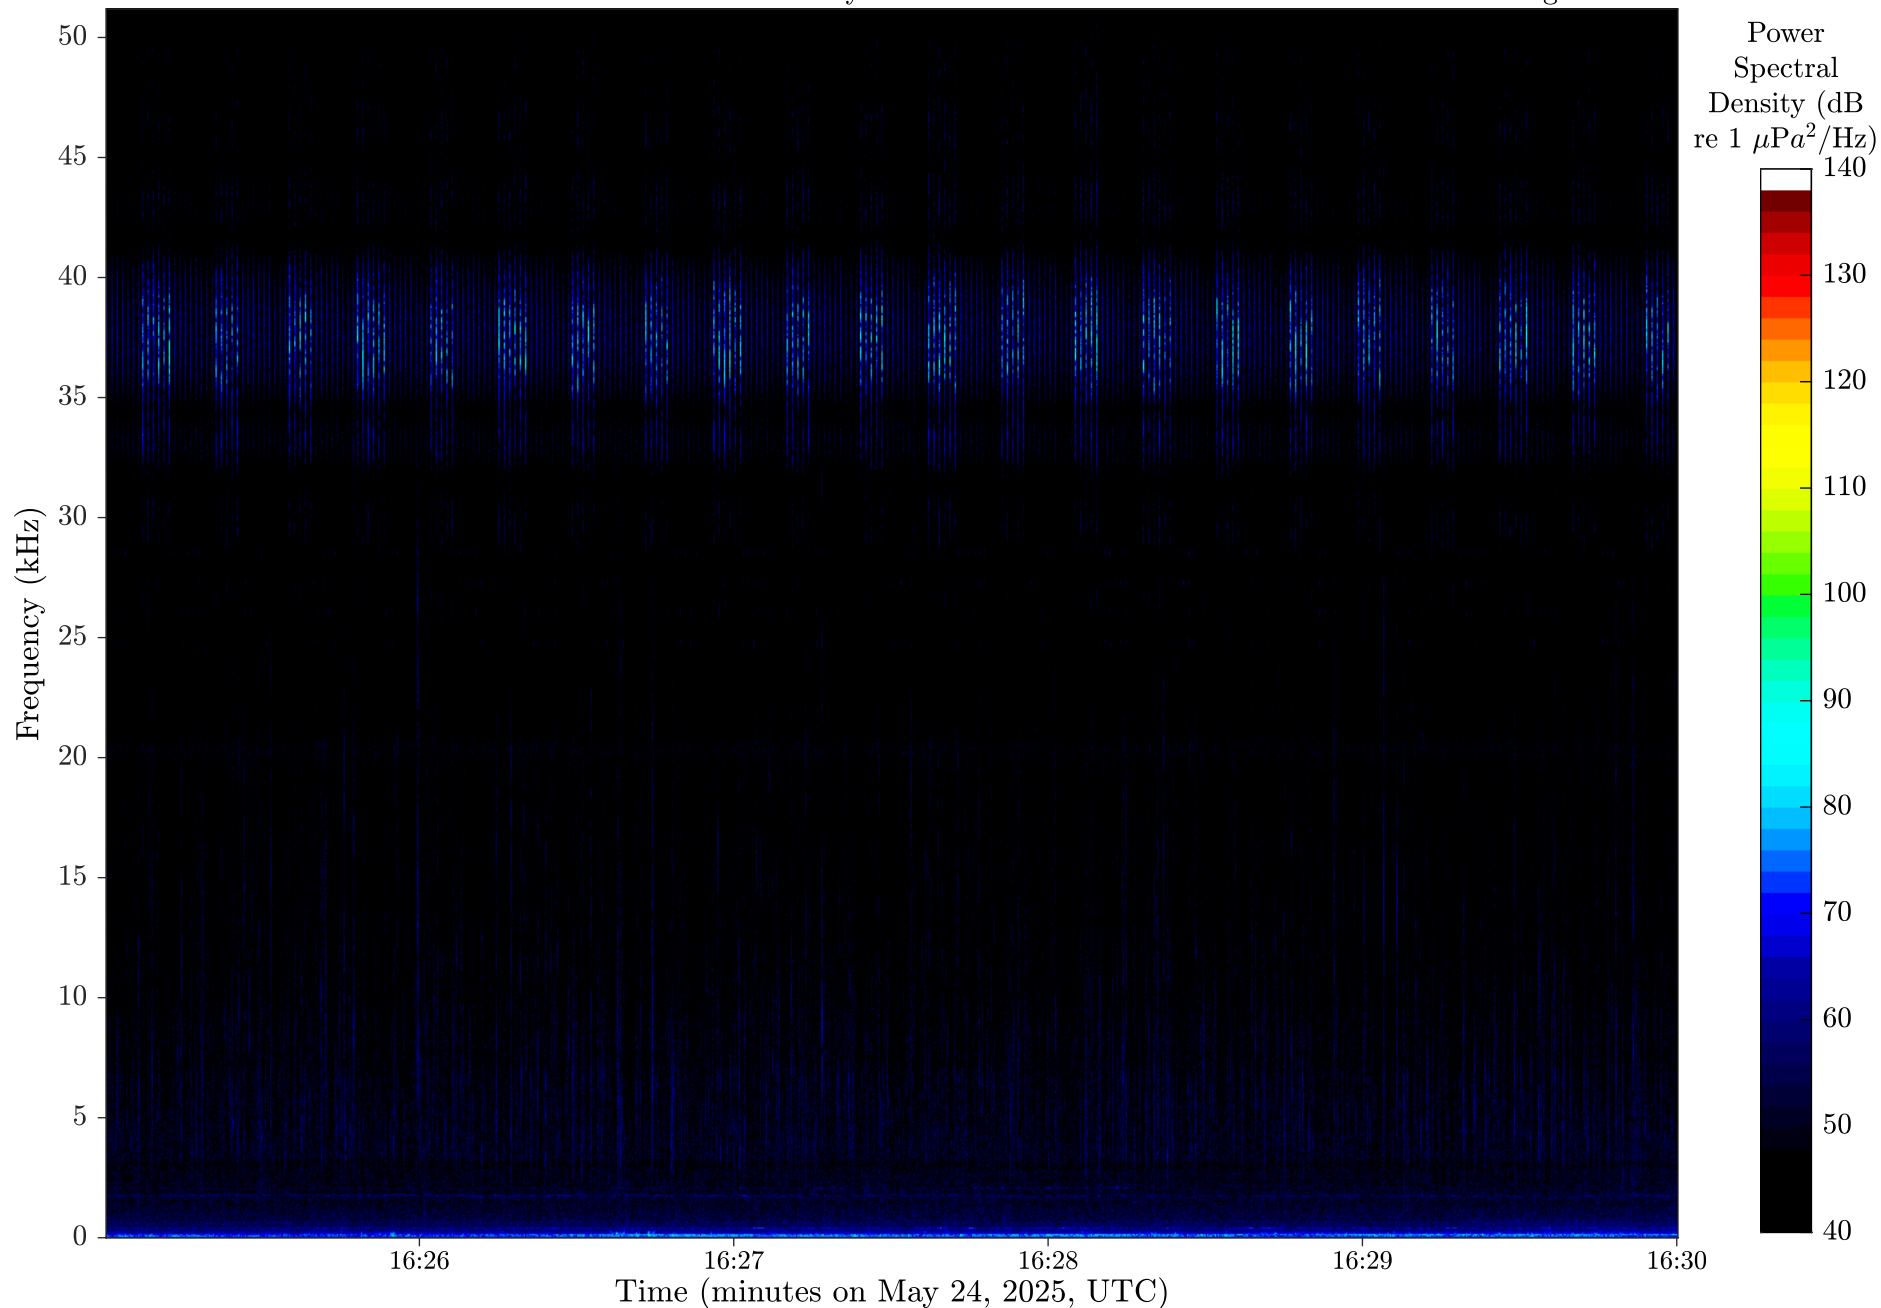


Comments: 29.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:12 UTC

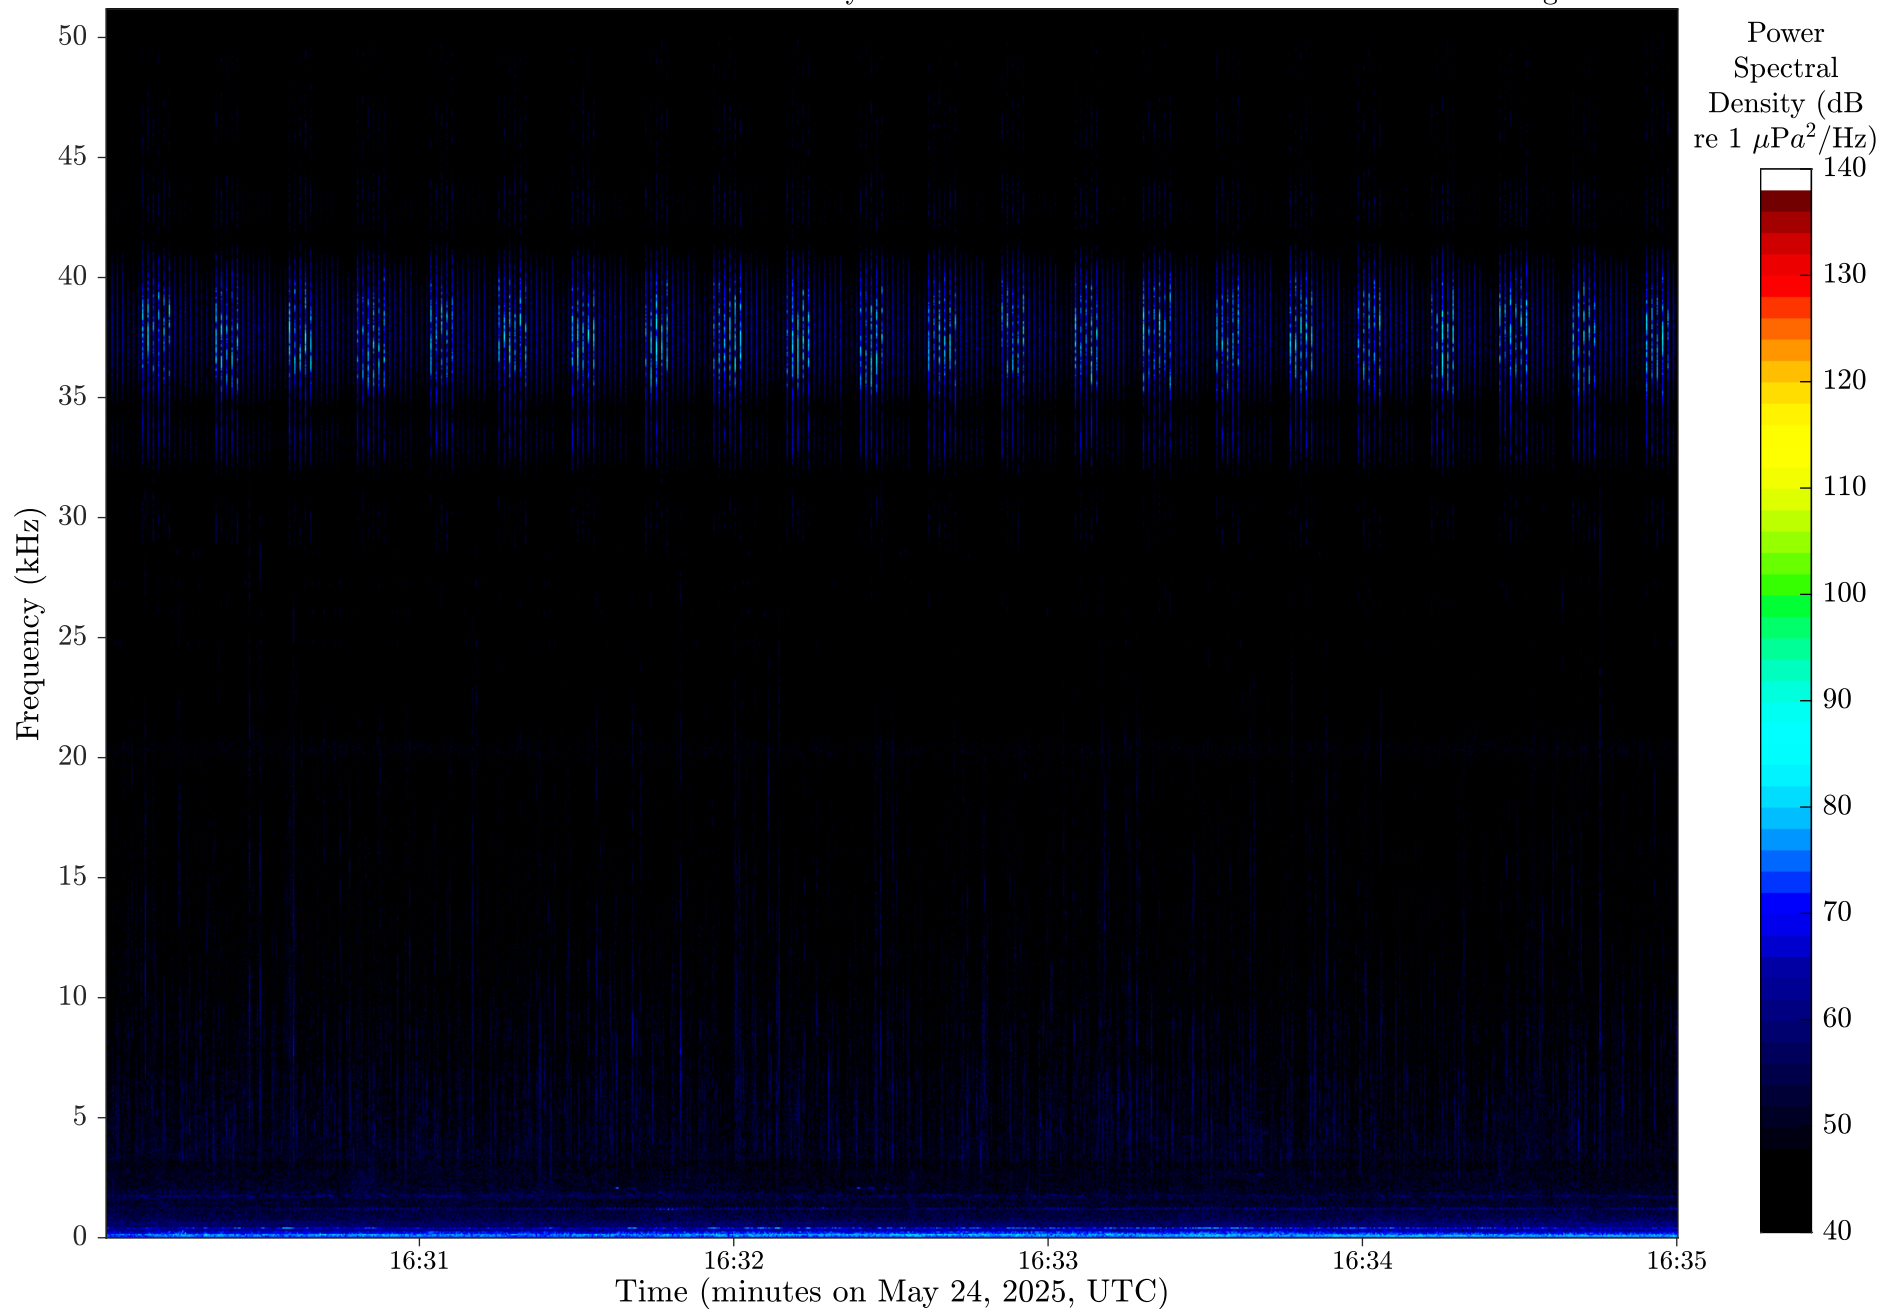


Comments: 31.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:20 UTC

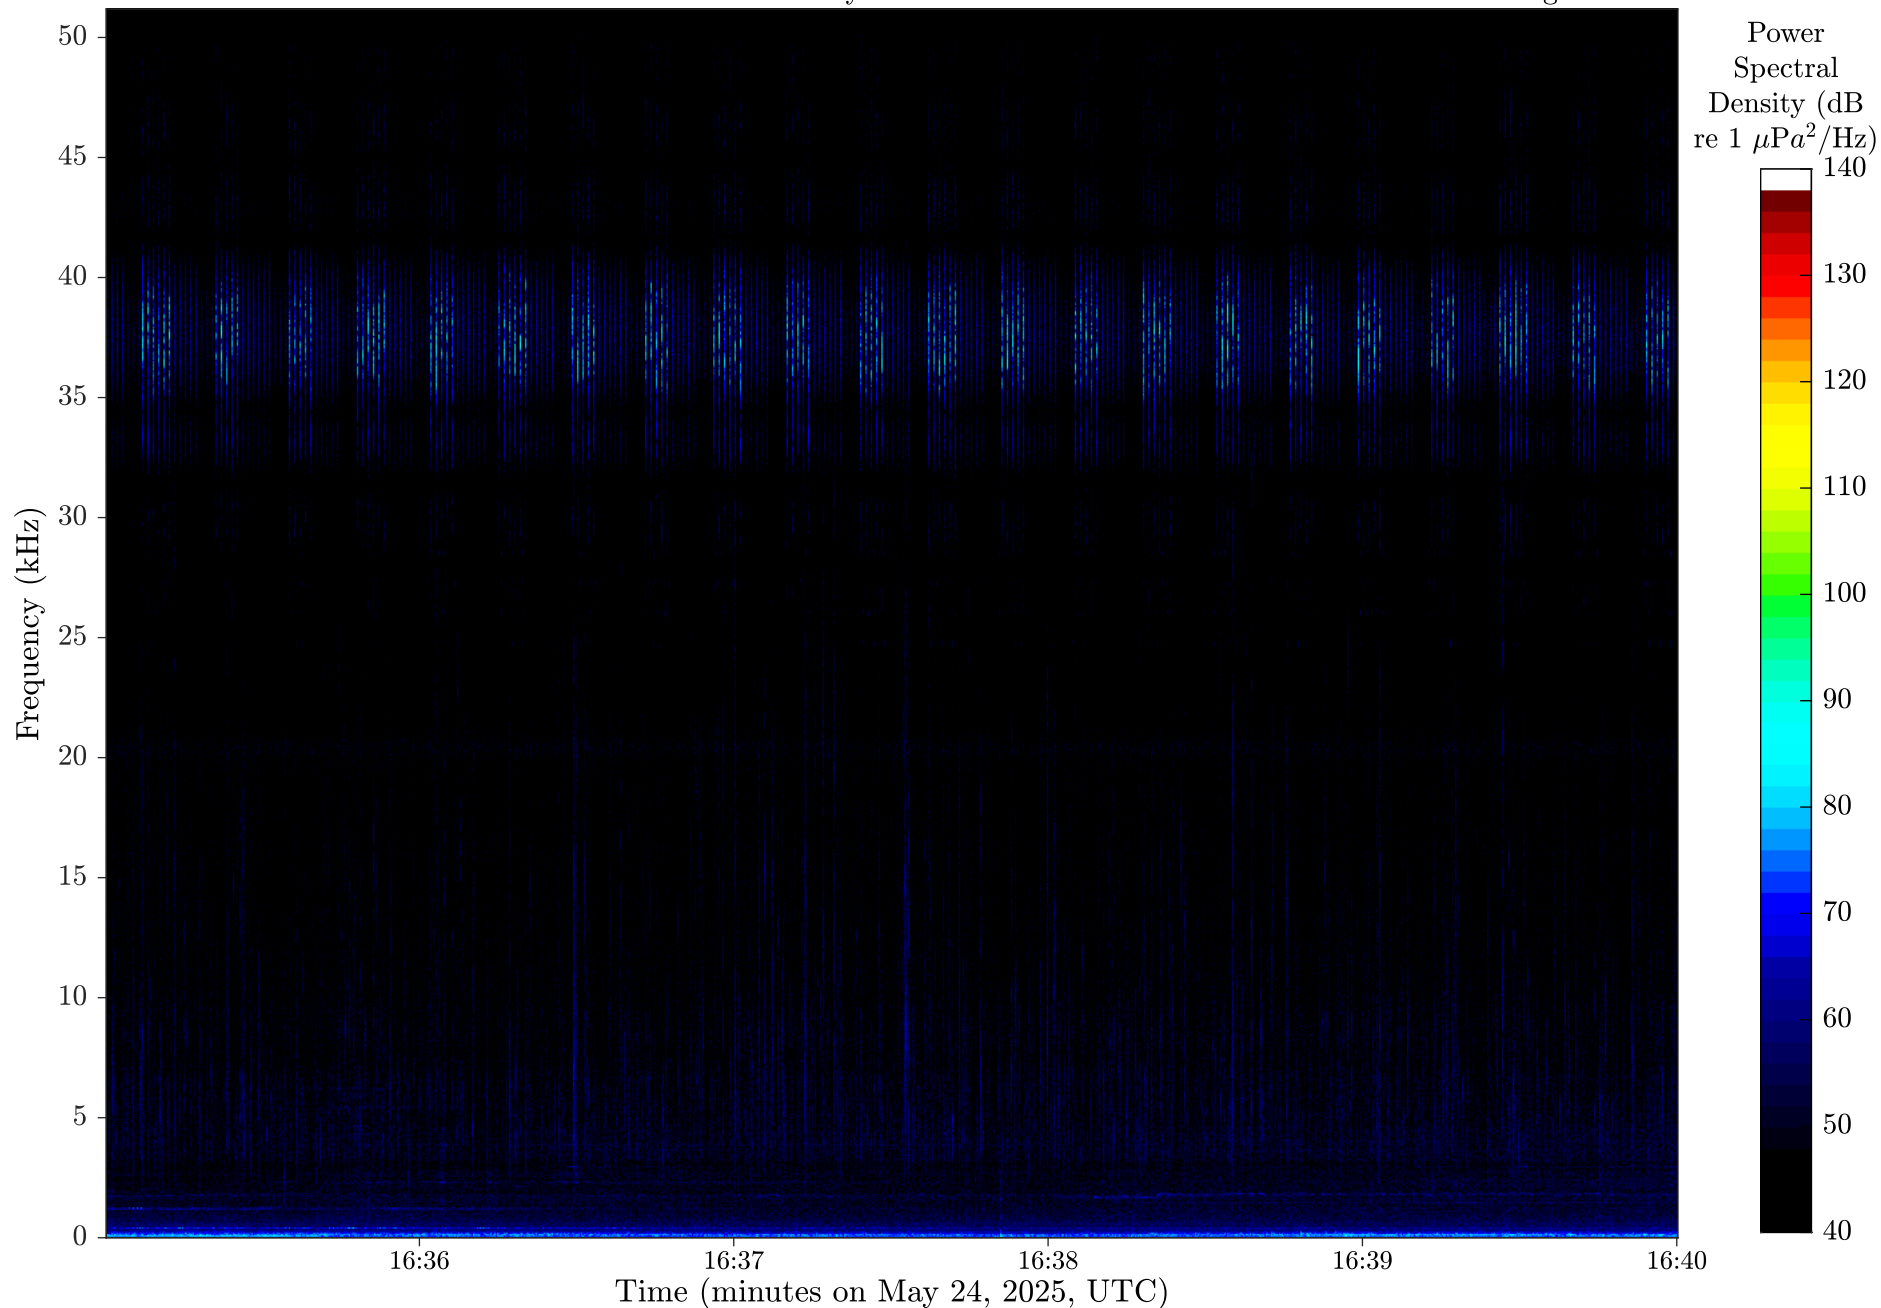


Comments: 30.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:36:27 UTC

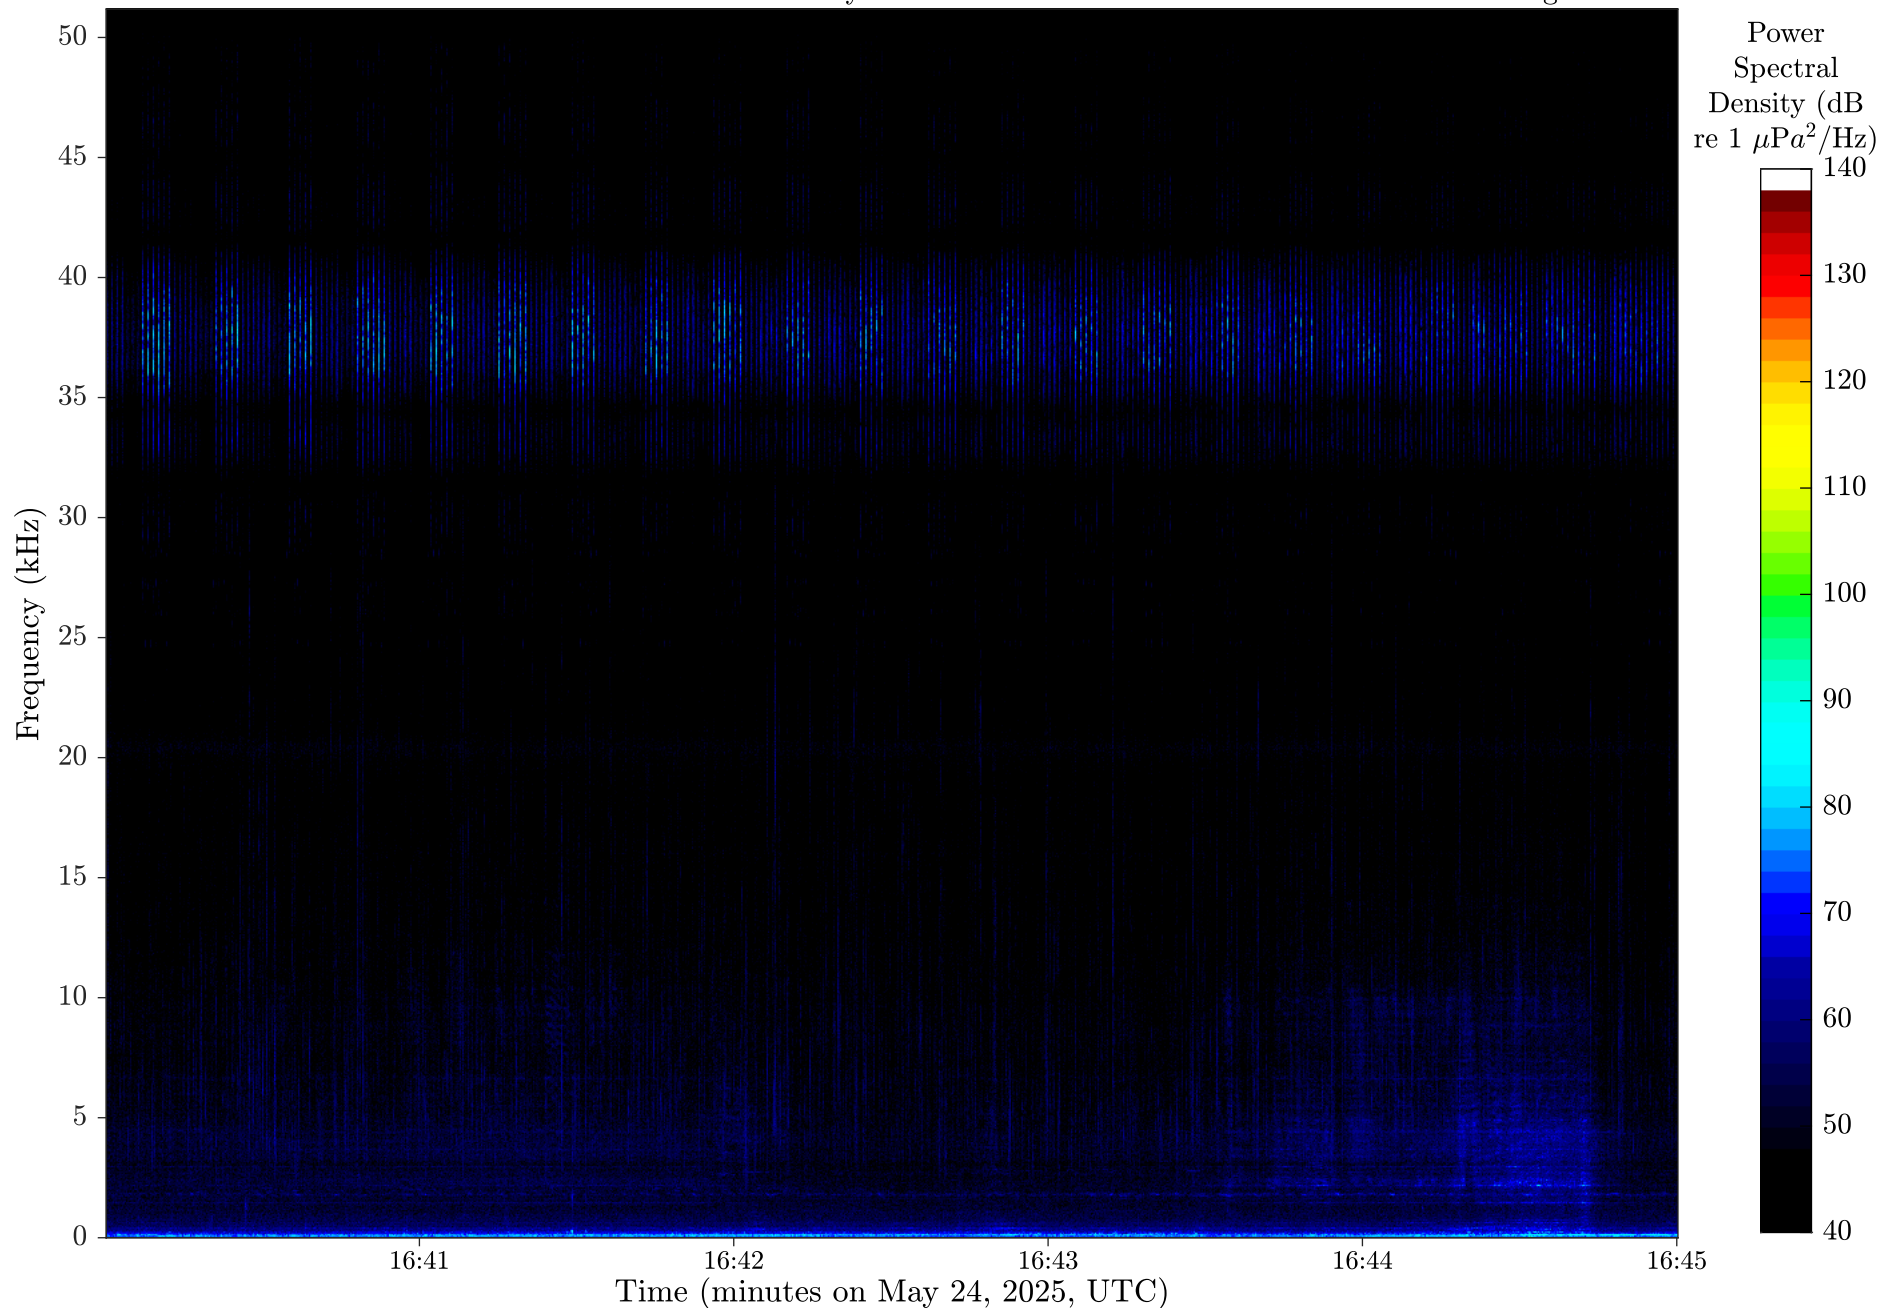

Comments: 29.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:36:34 UTC

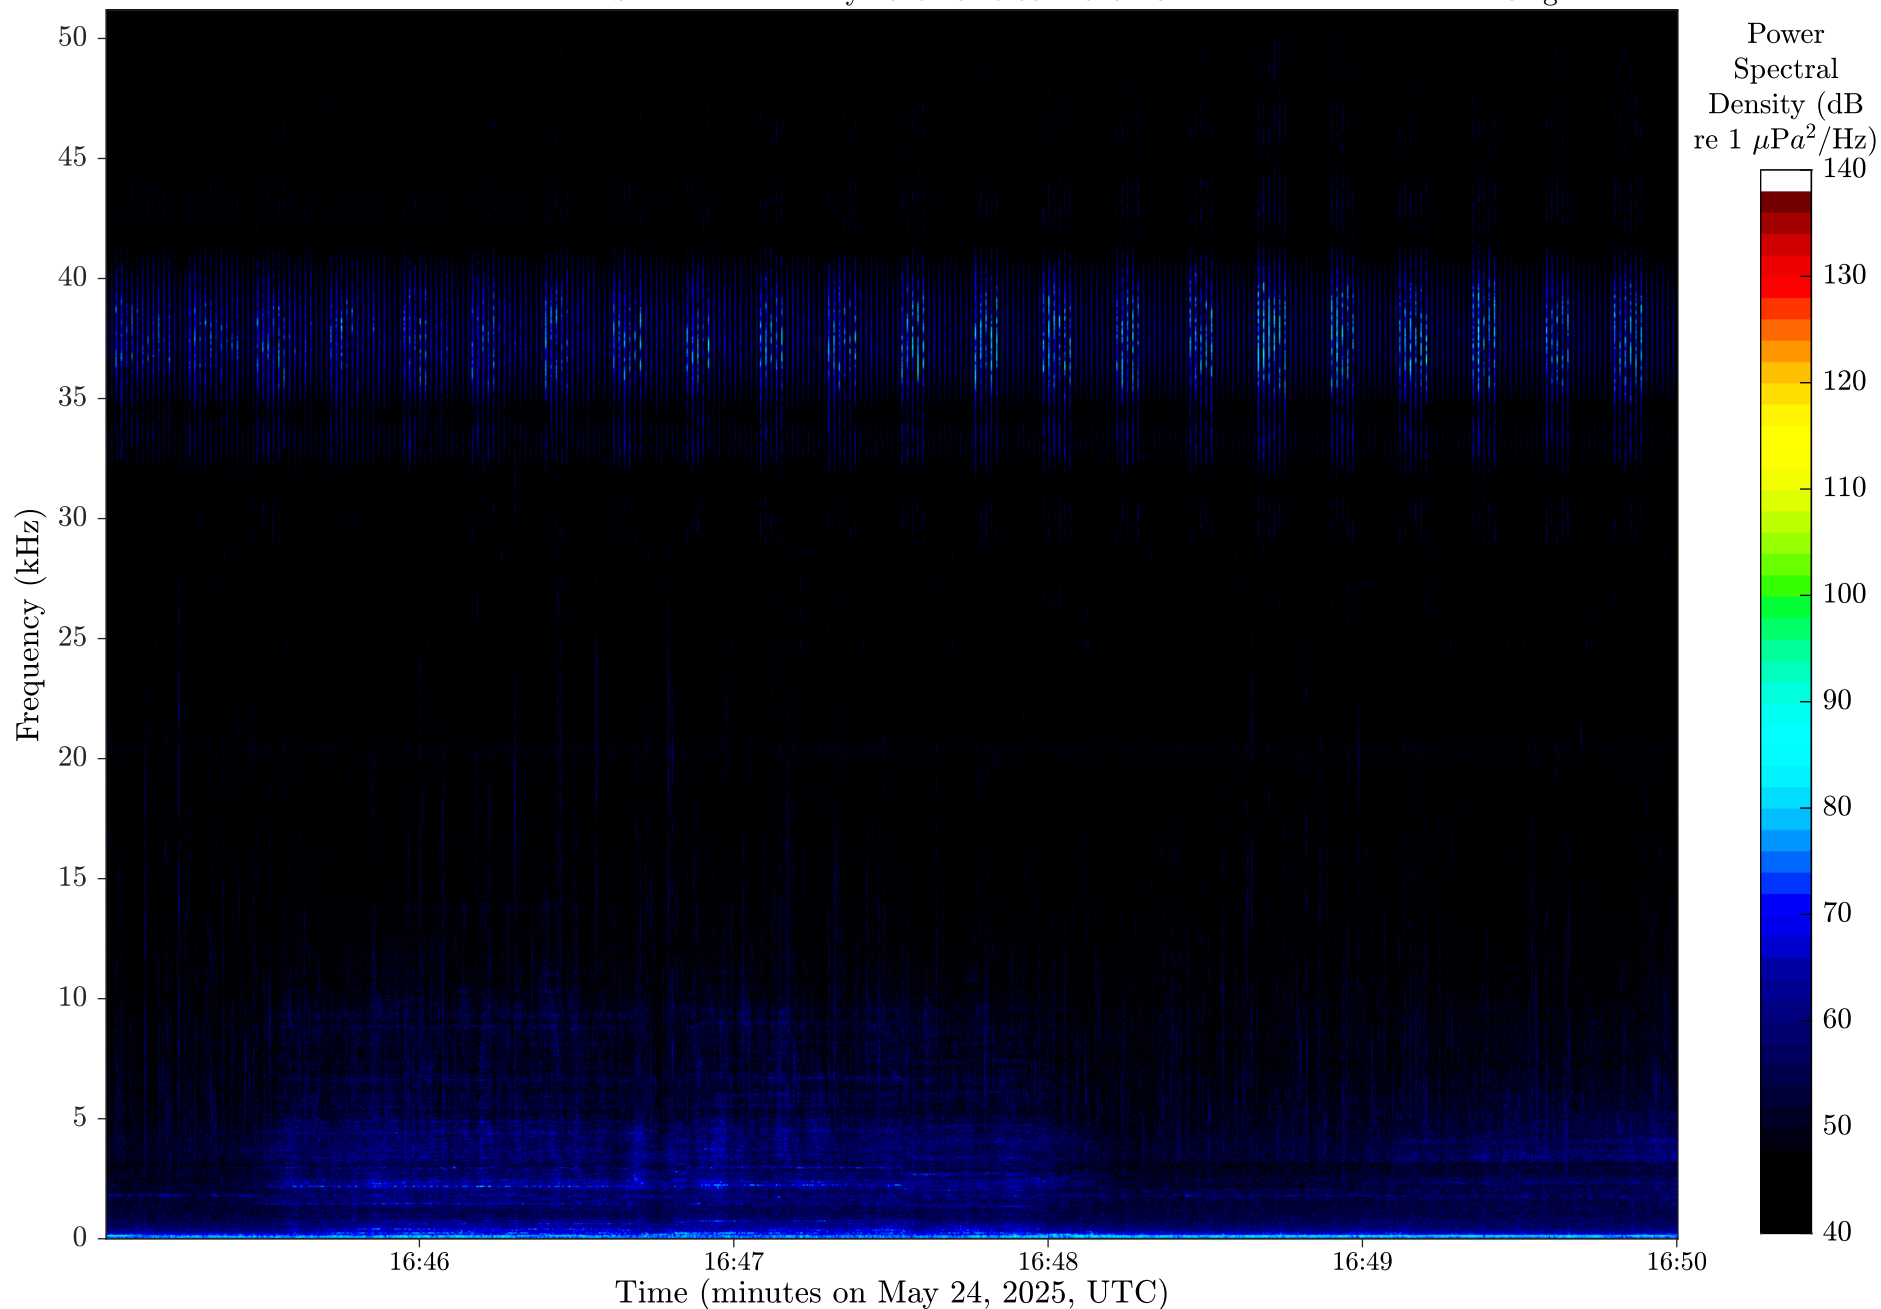

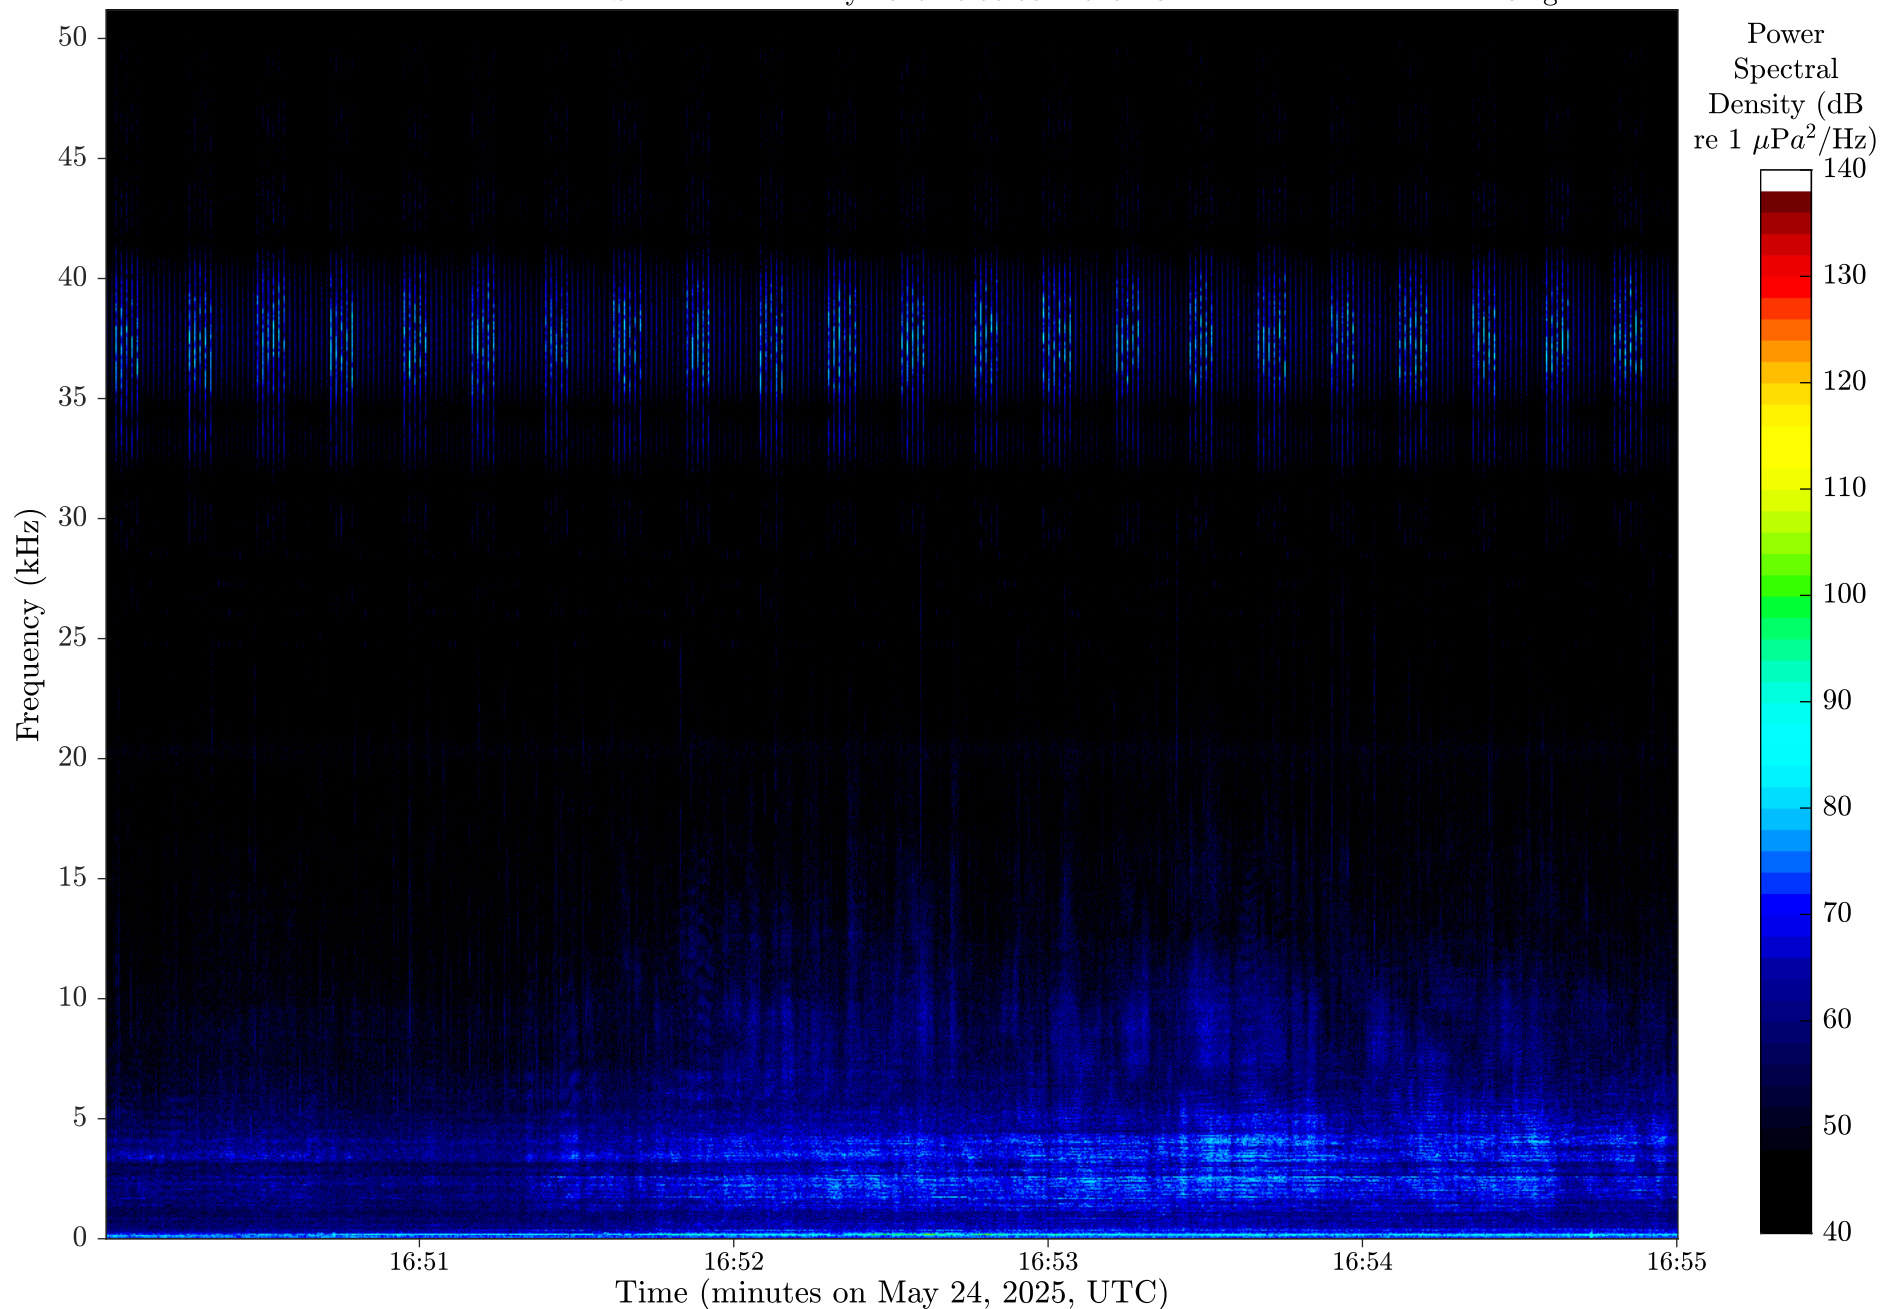


Comments: 26.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:48 UTC

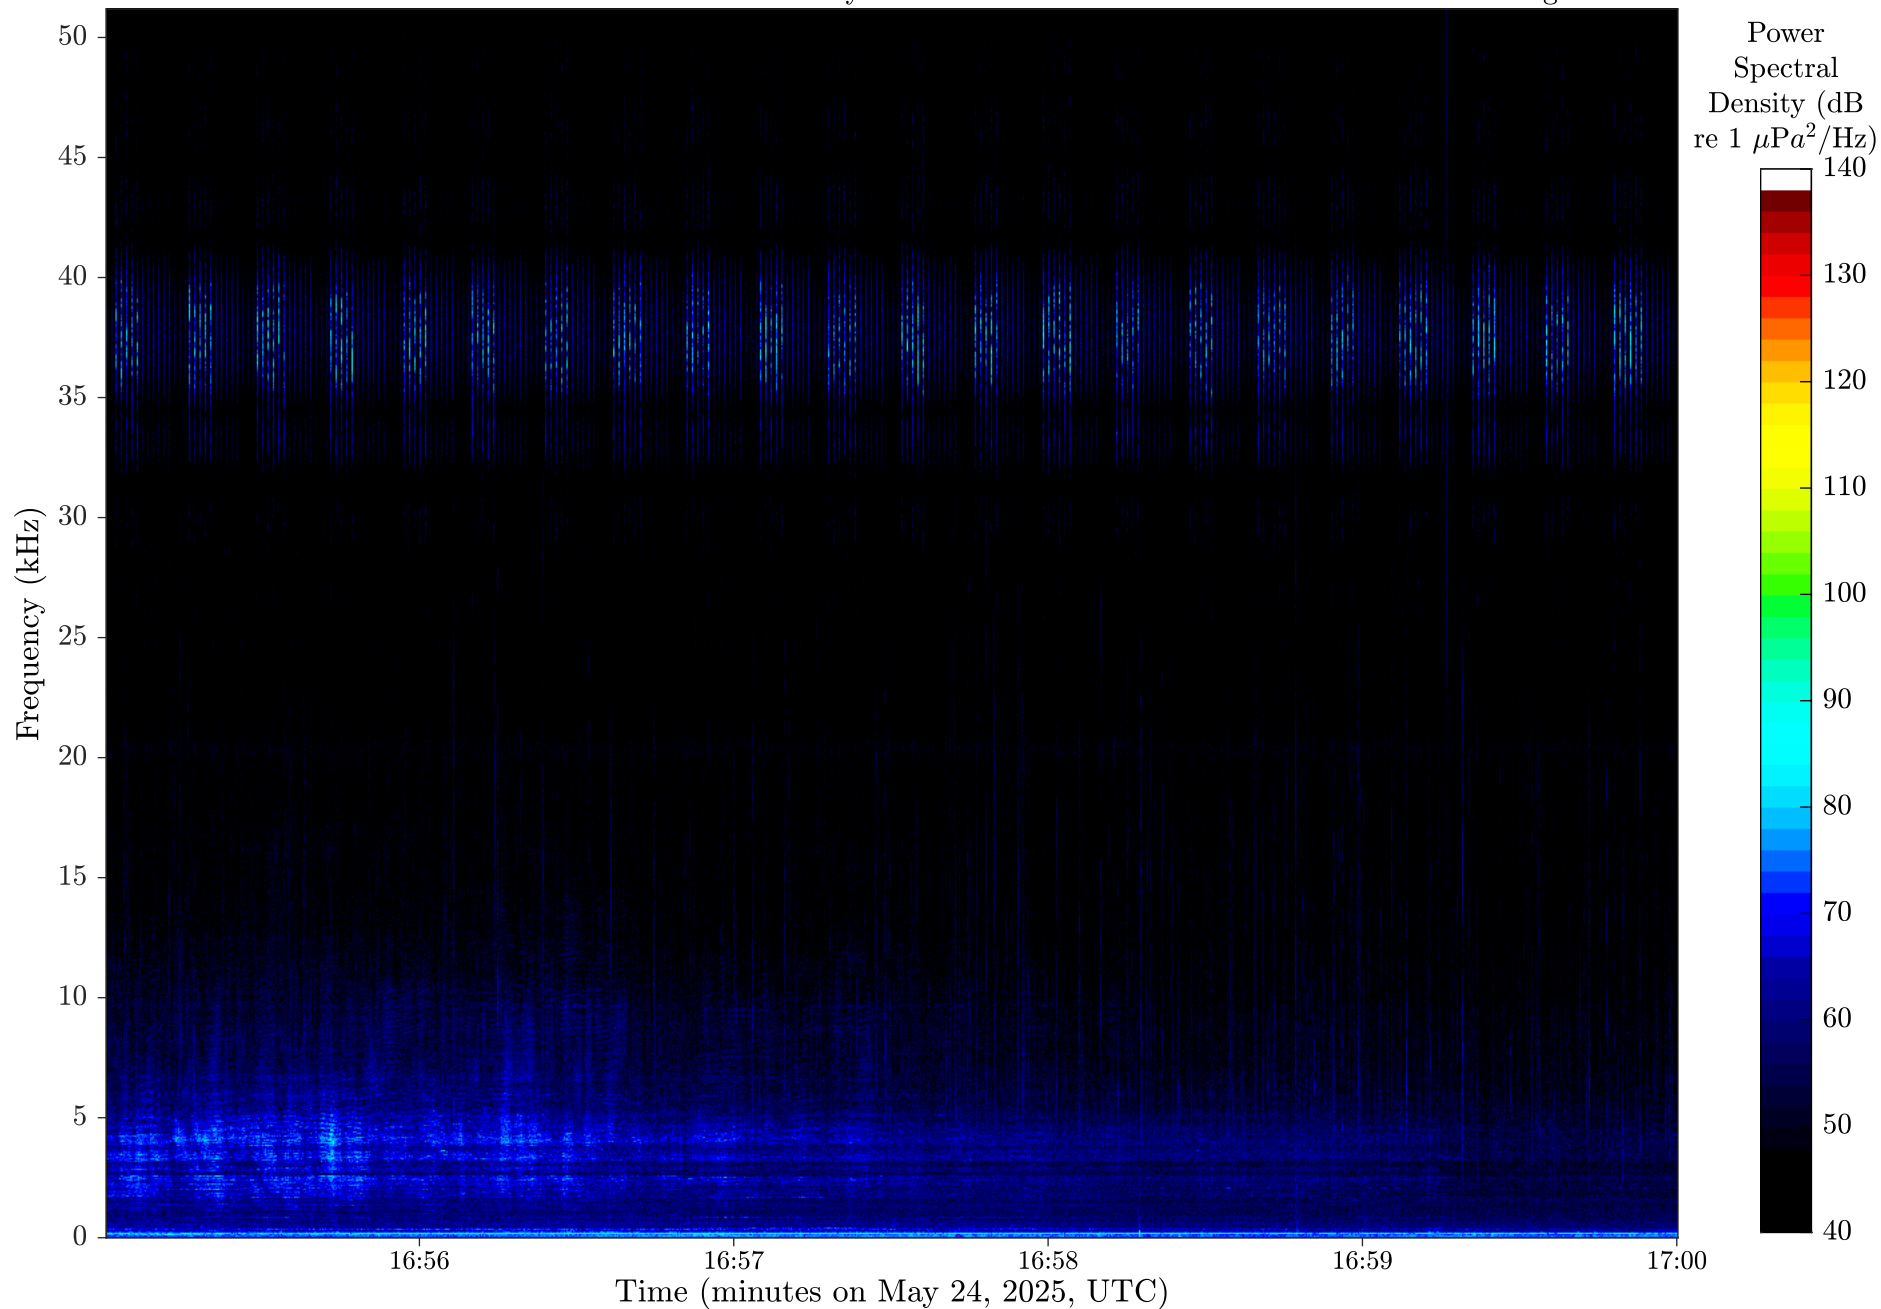


Comments: 28.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:55 UTC

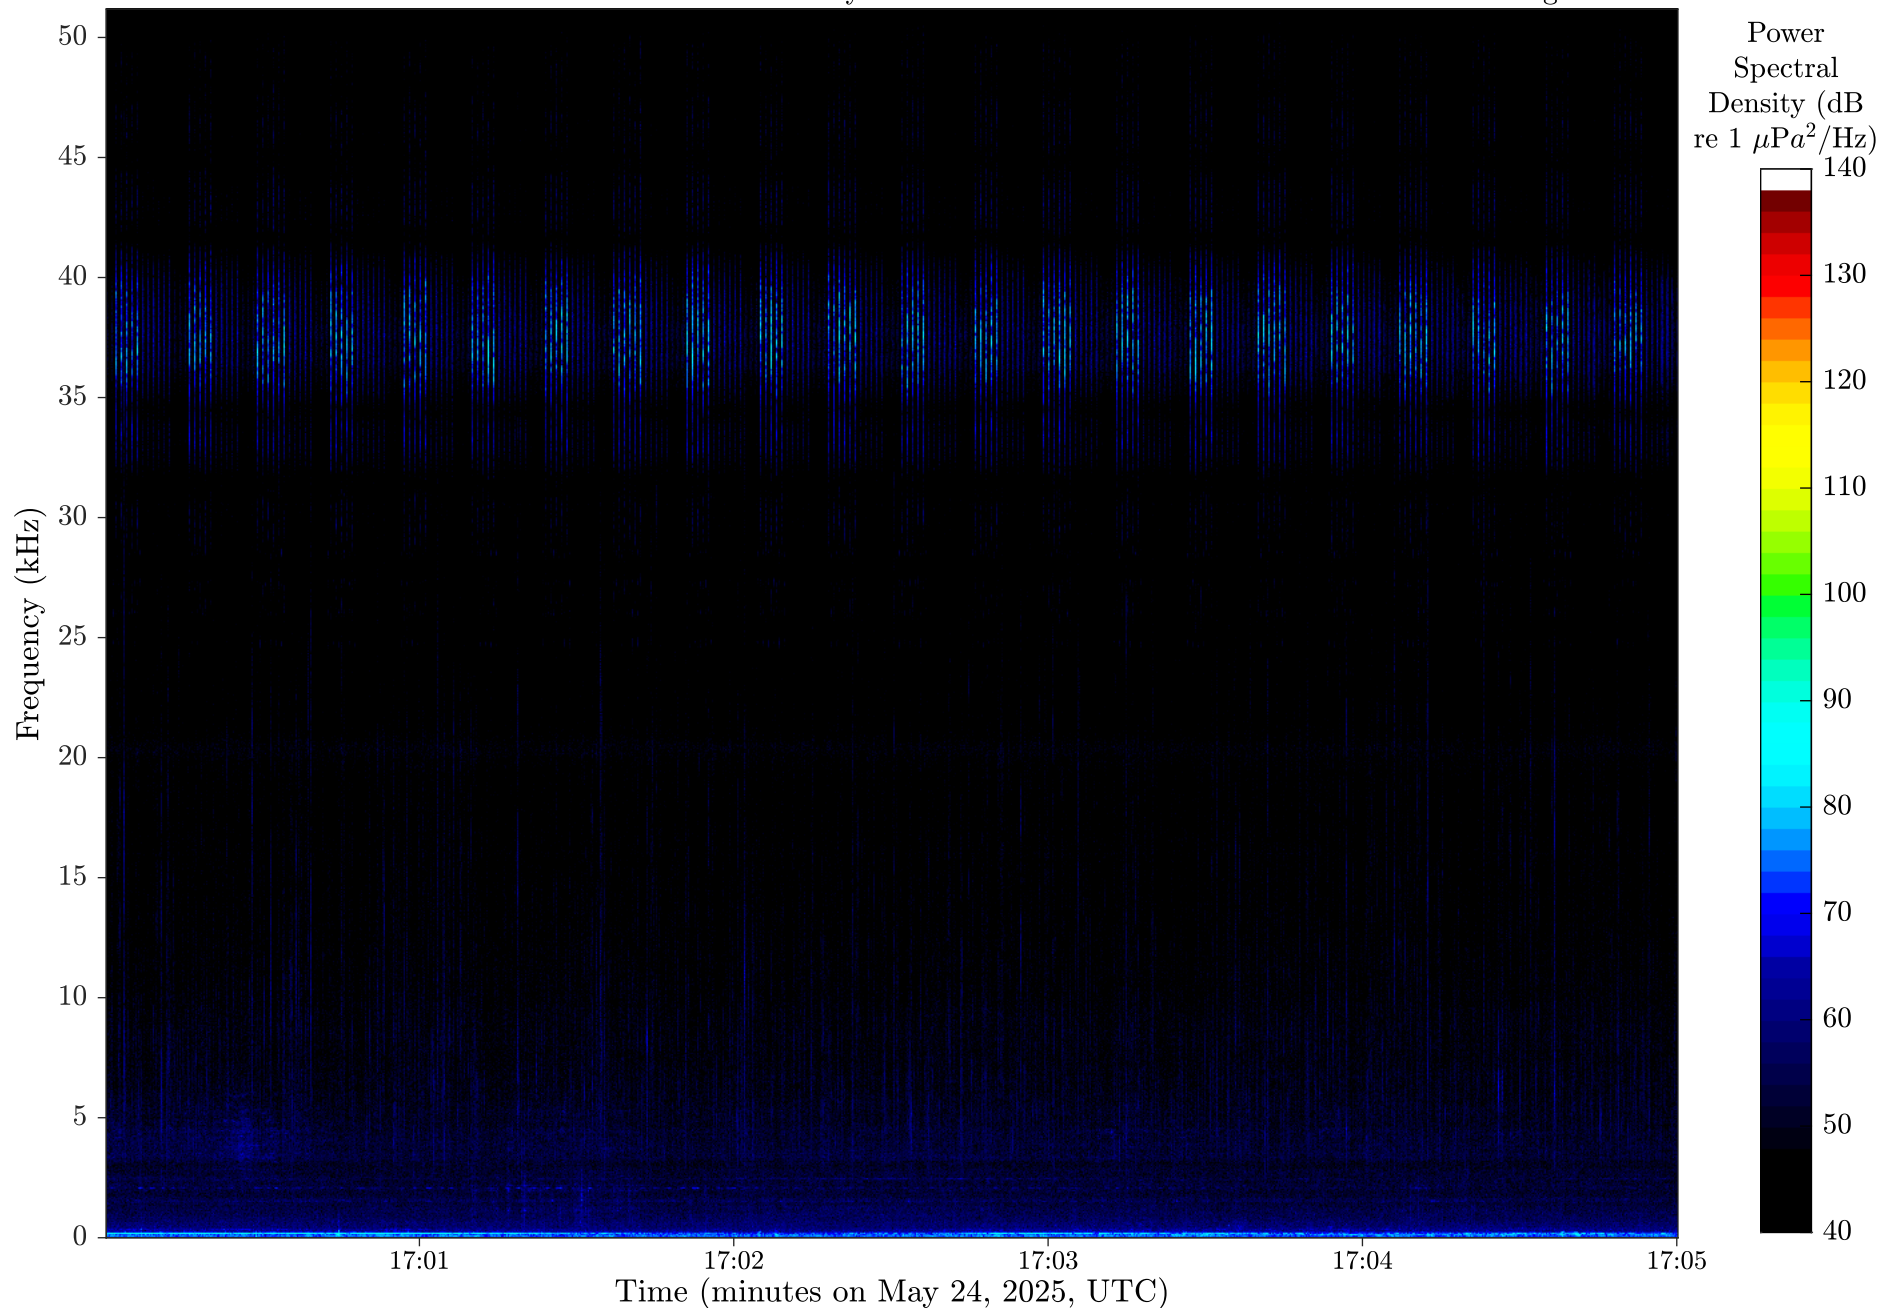


Comments: 28.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:03 UTC

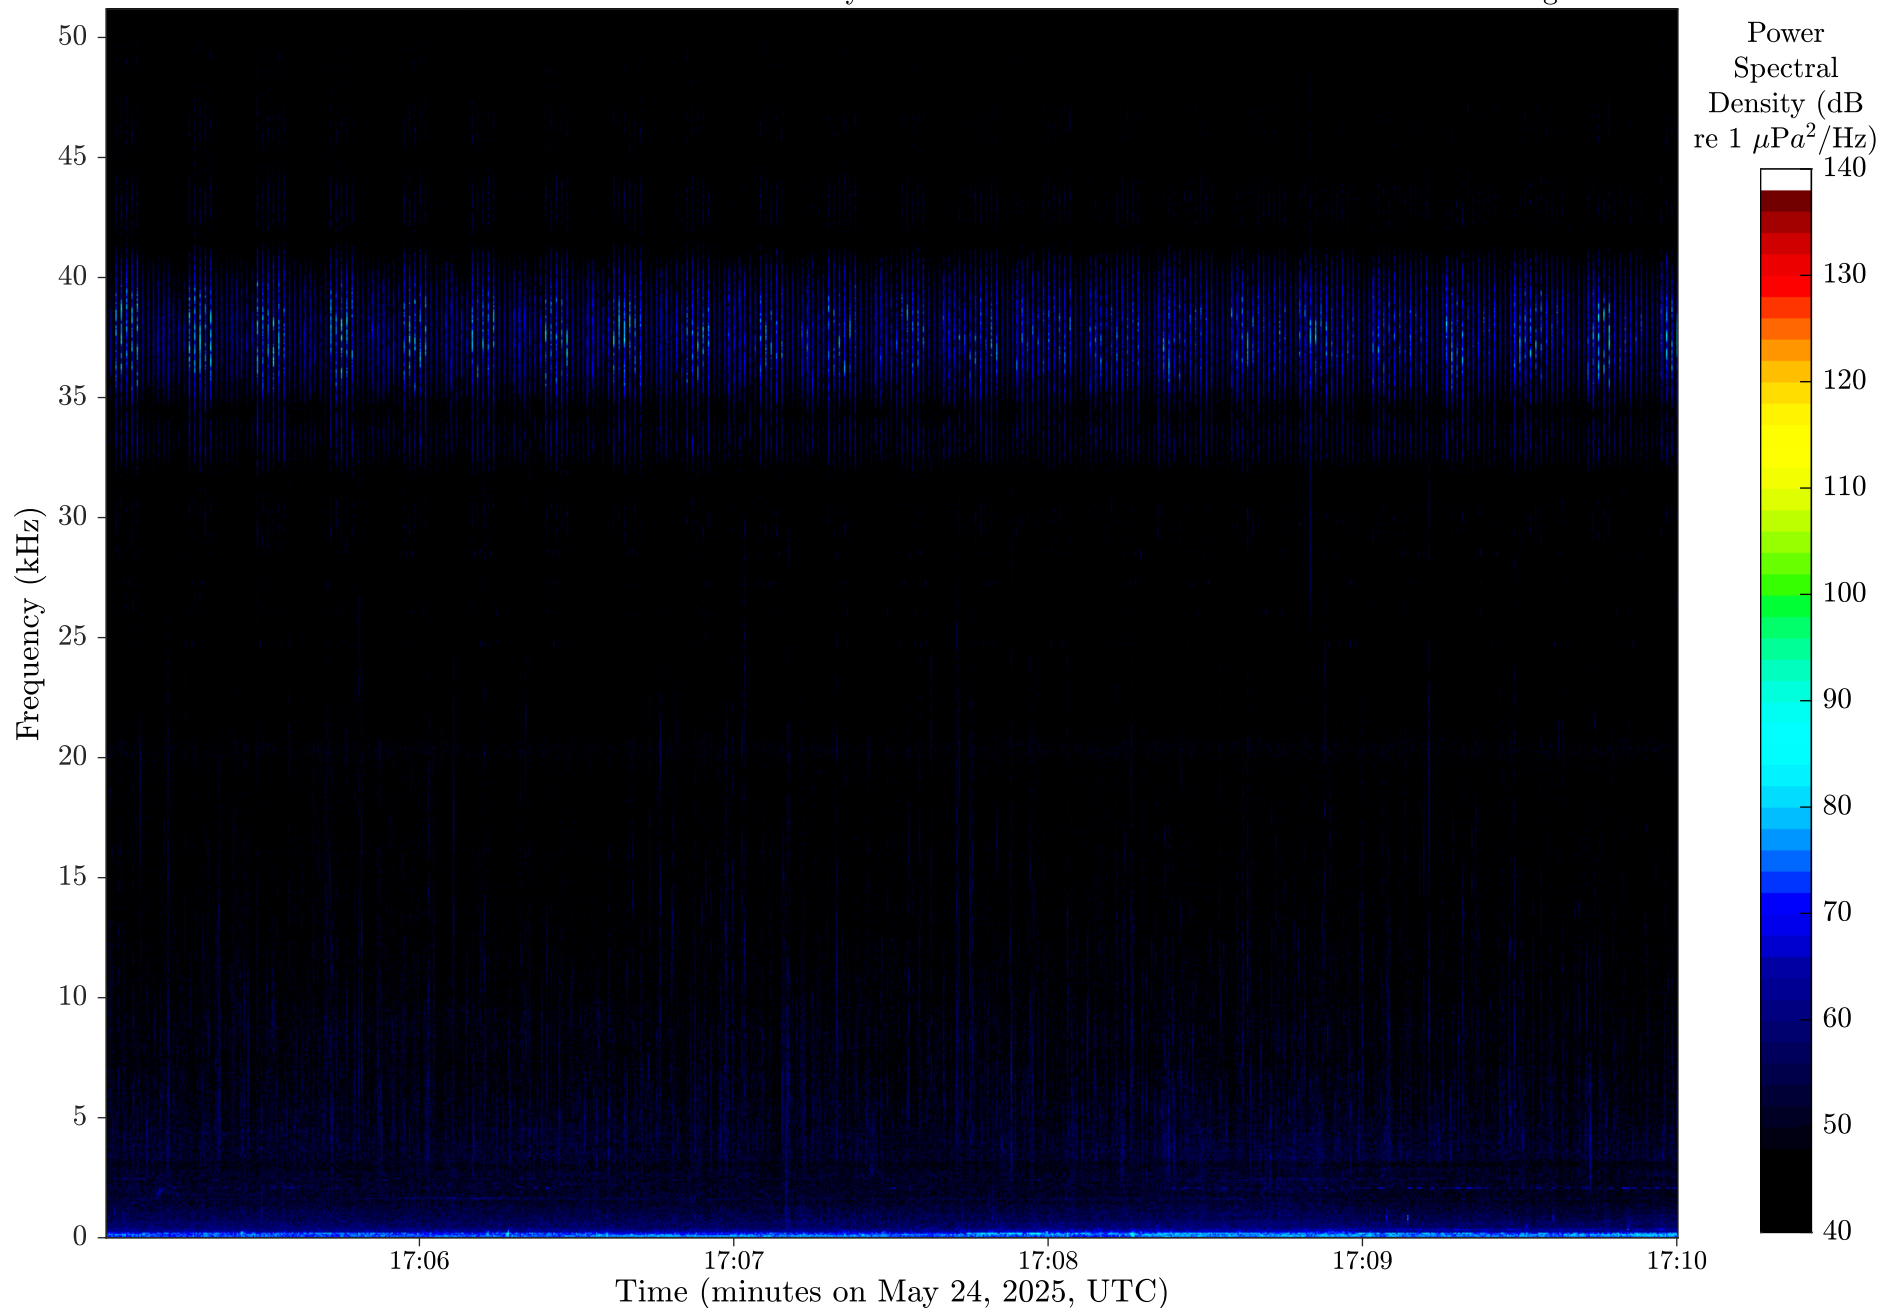


Comments: 28.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:10 UTC

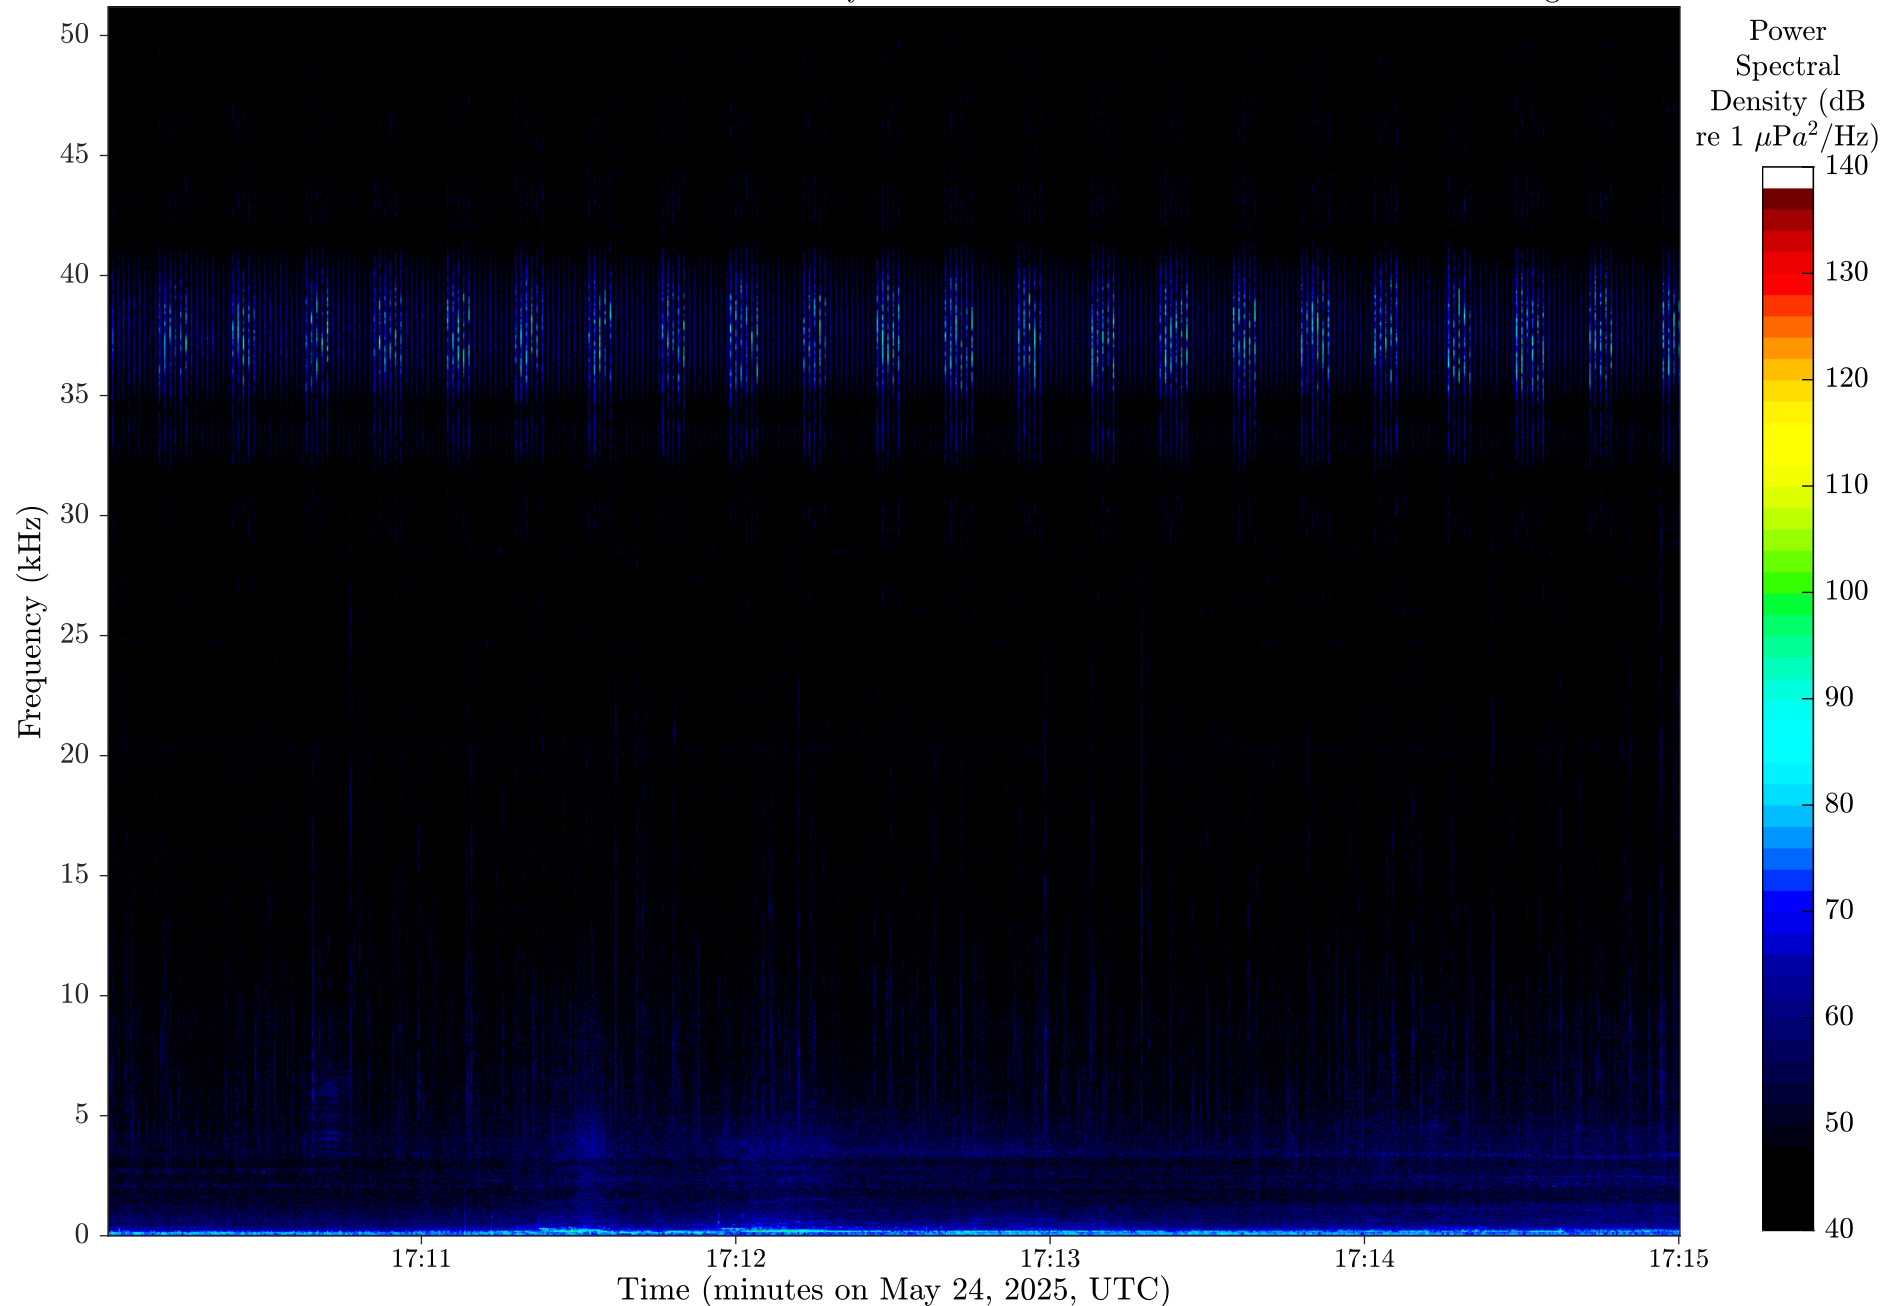


Comments: 30.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:18 UTC

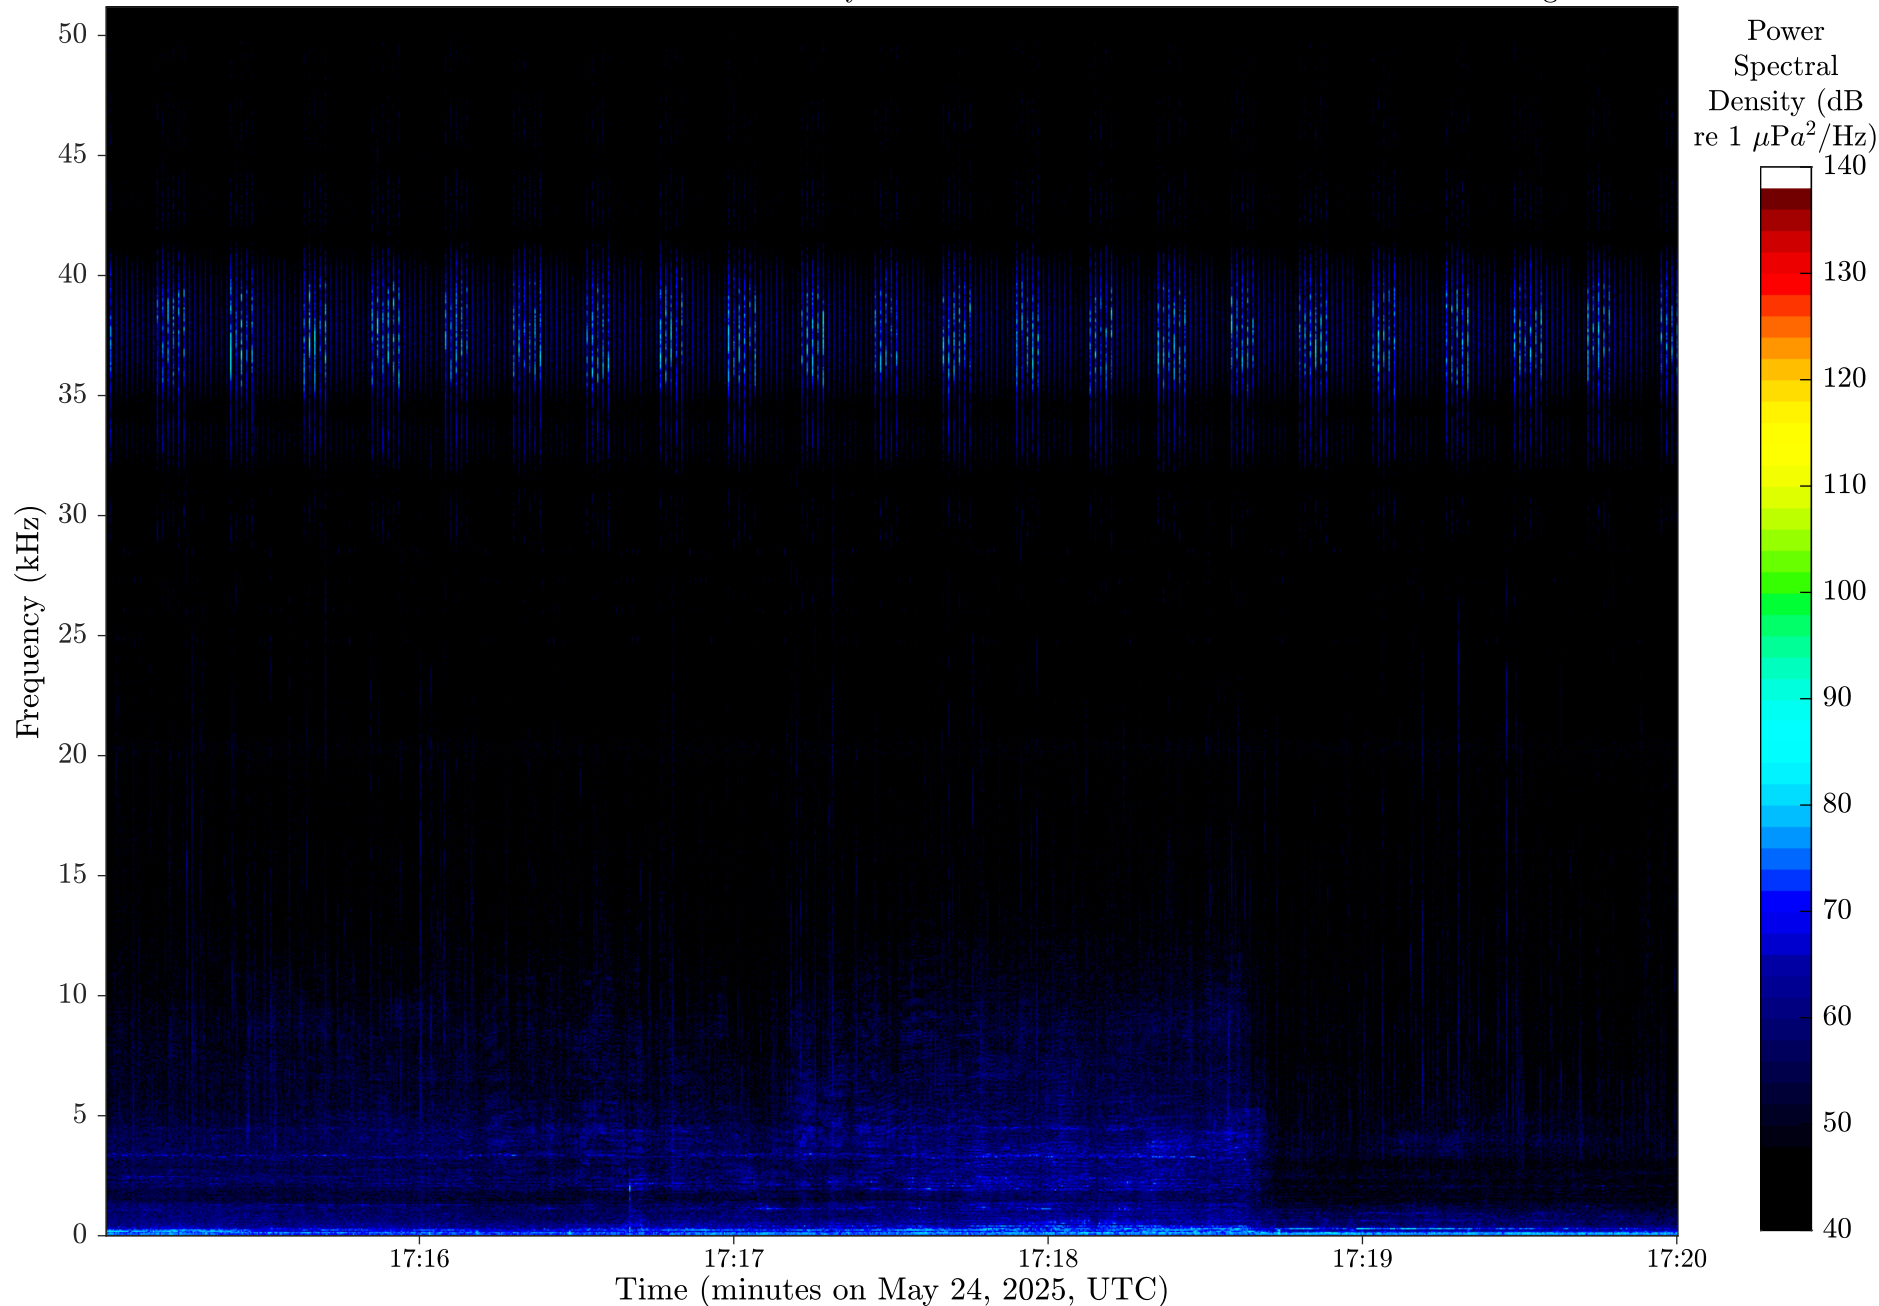


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:25 UTC

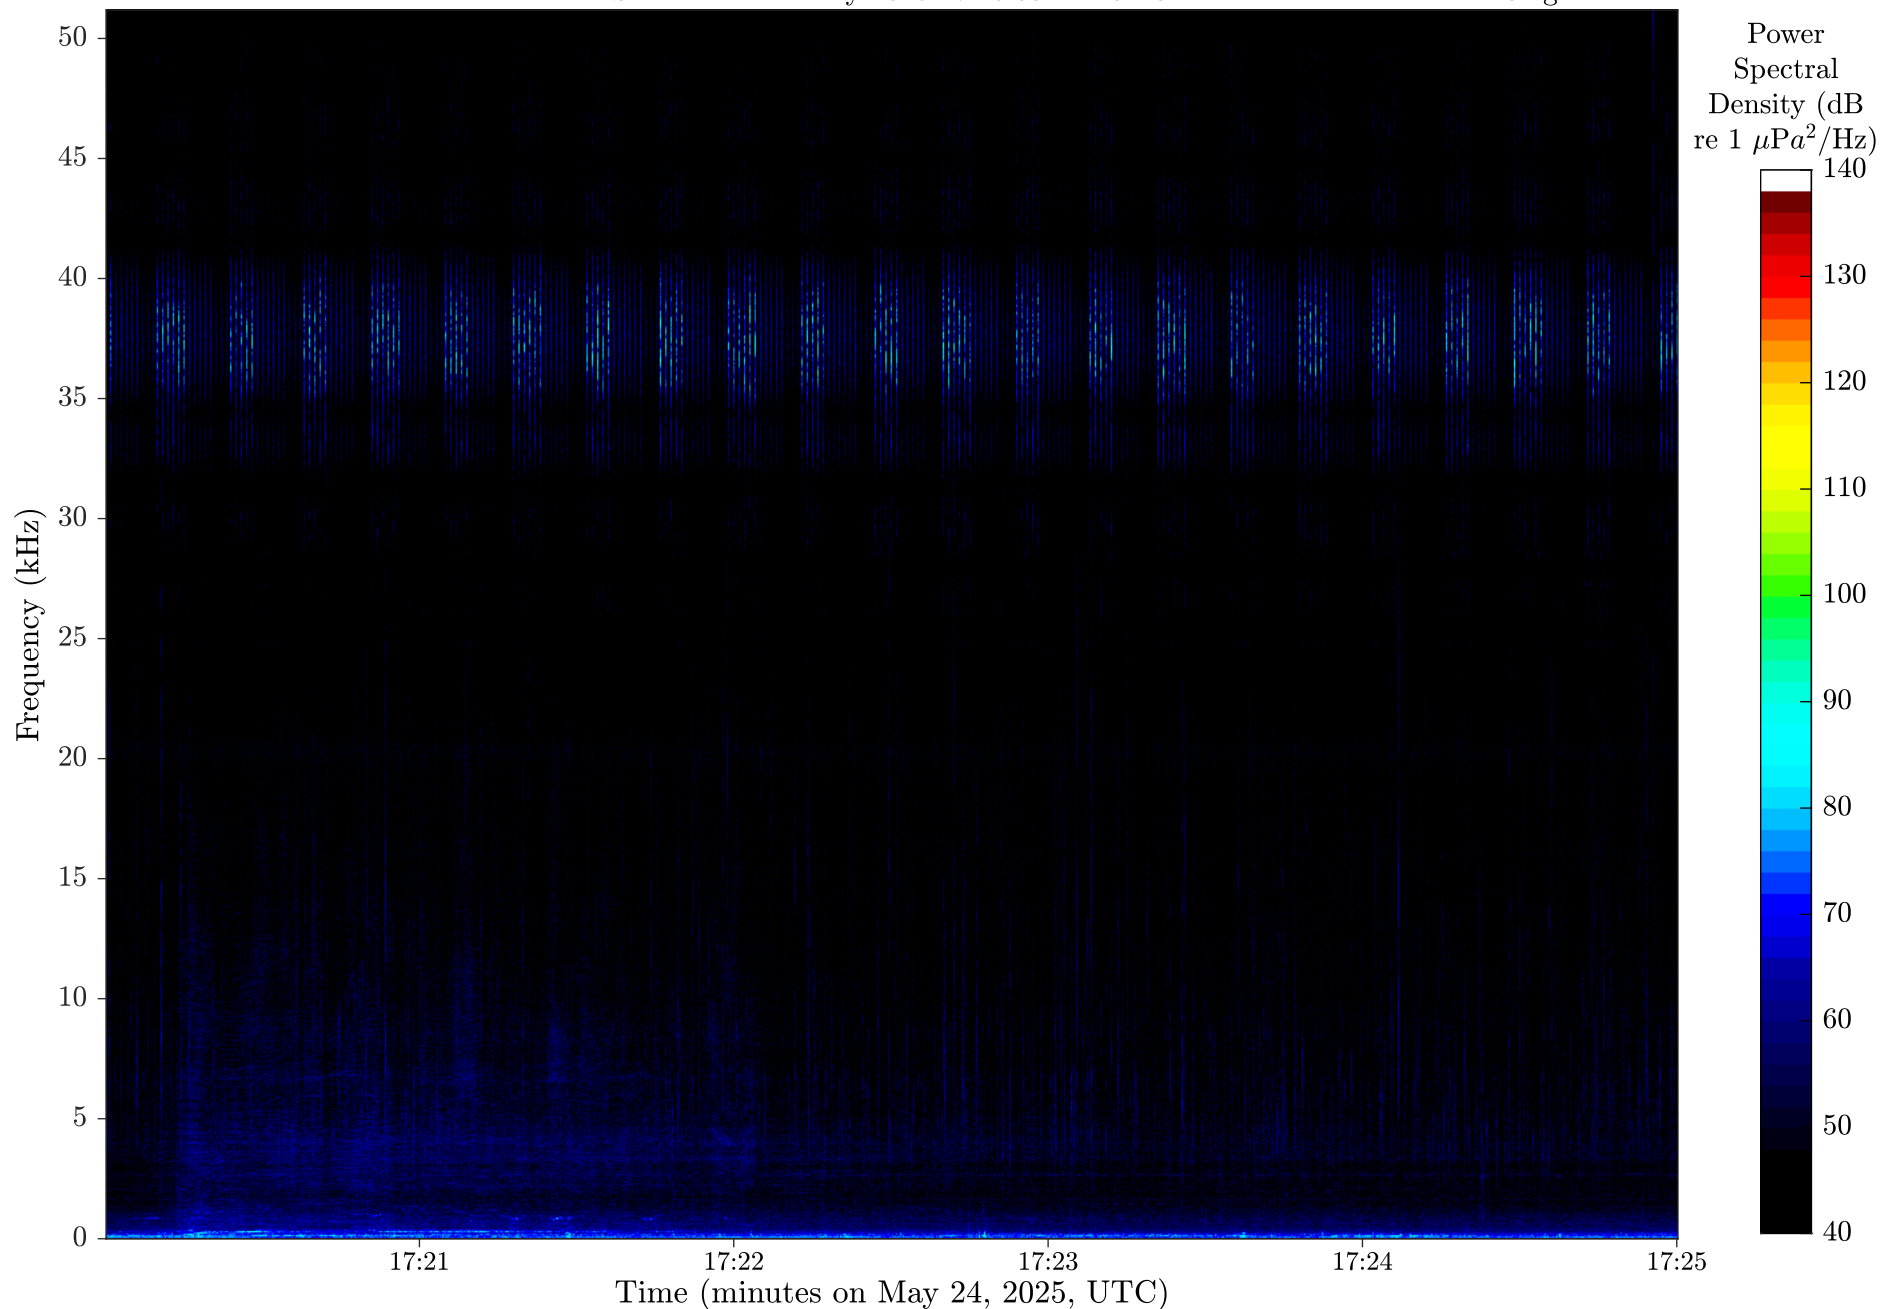


Comments: 32.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:32 UTC

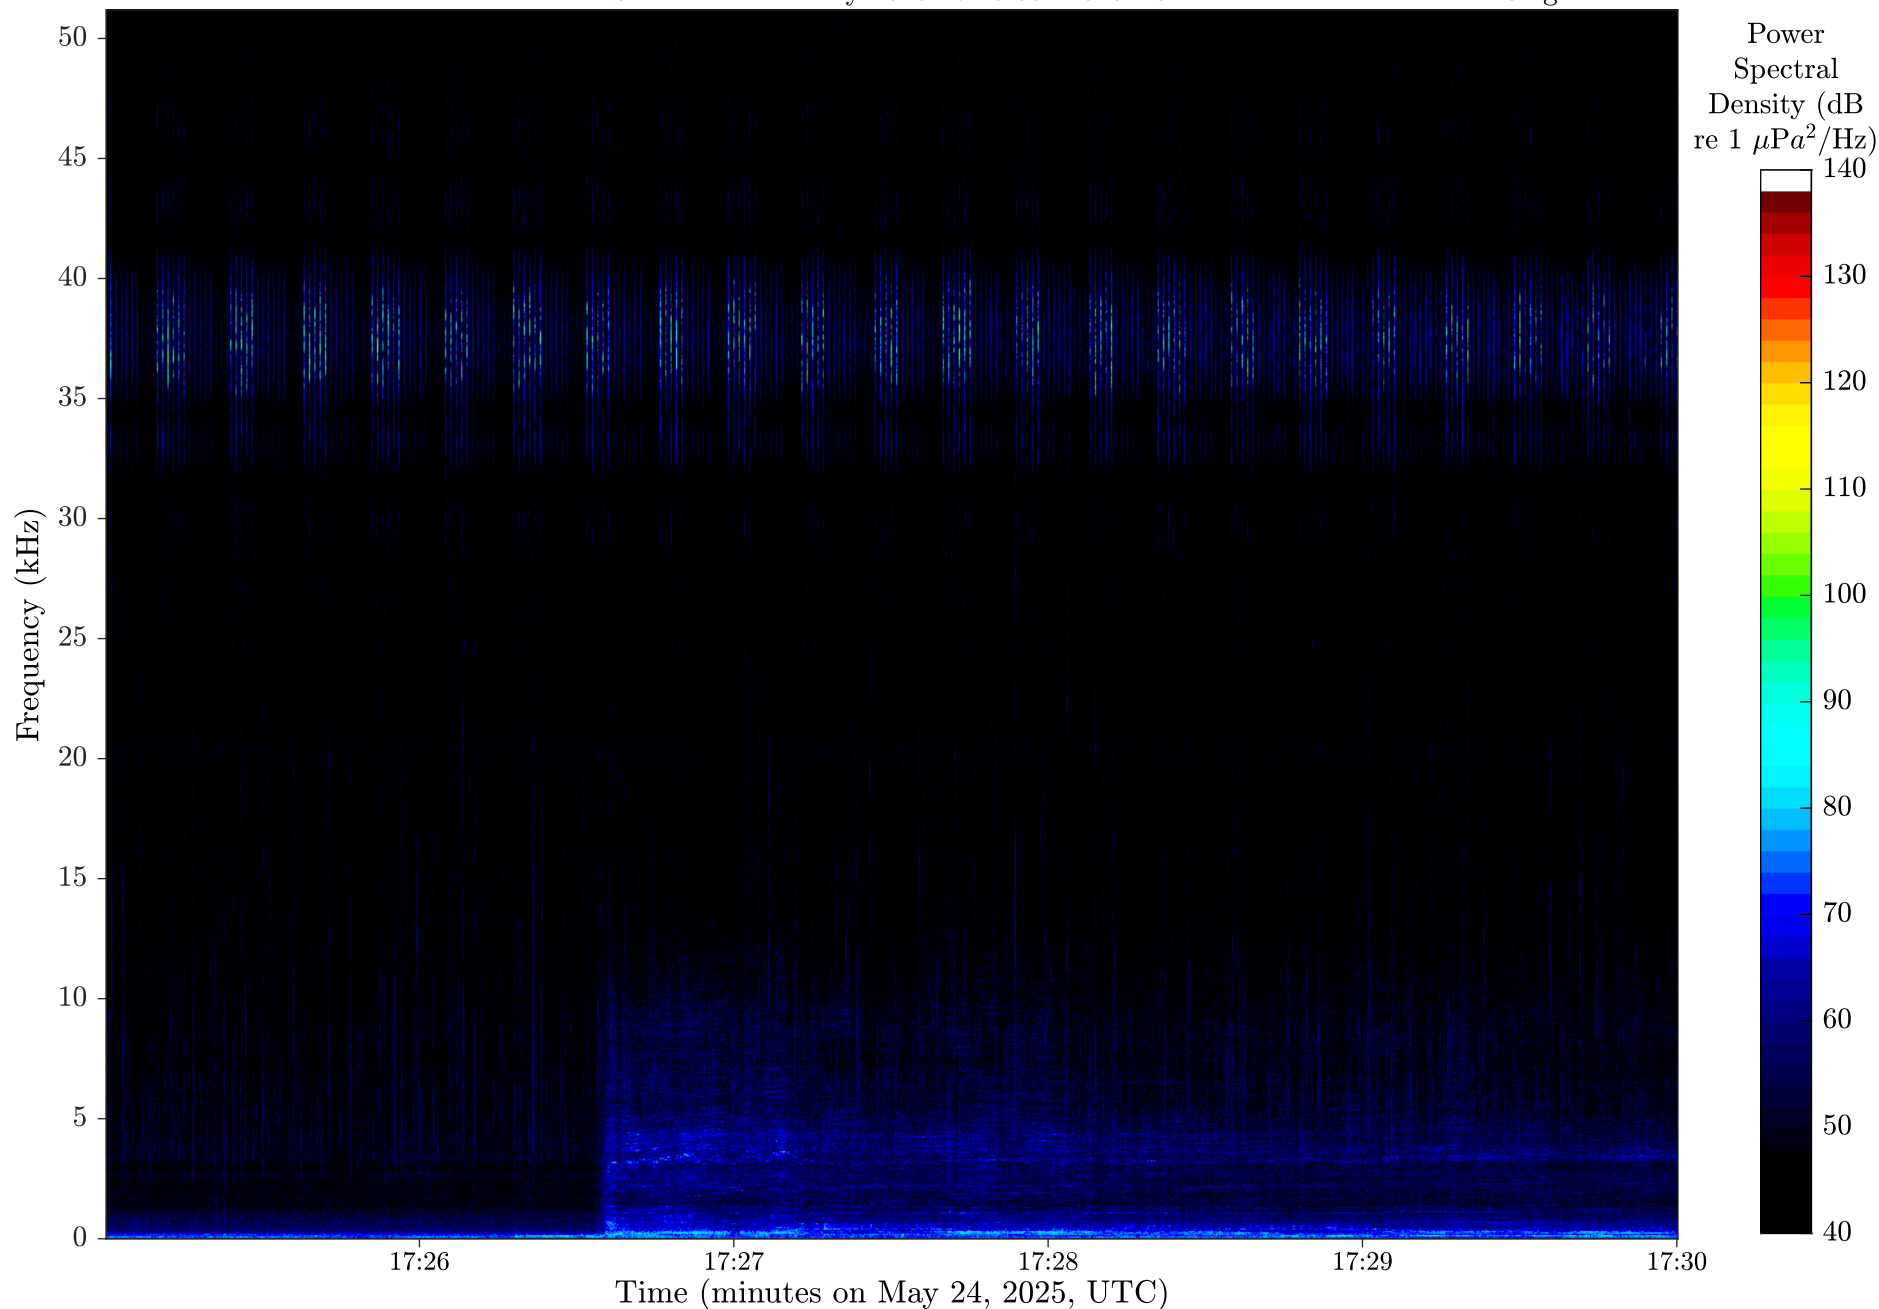


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:39 UTC

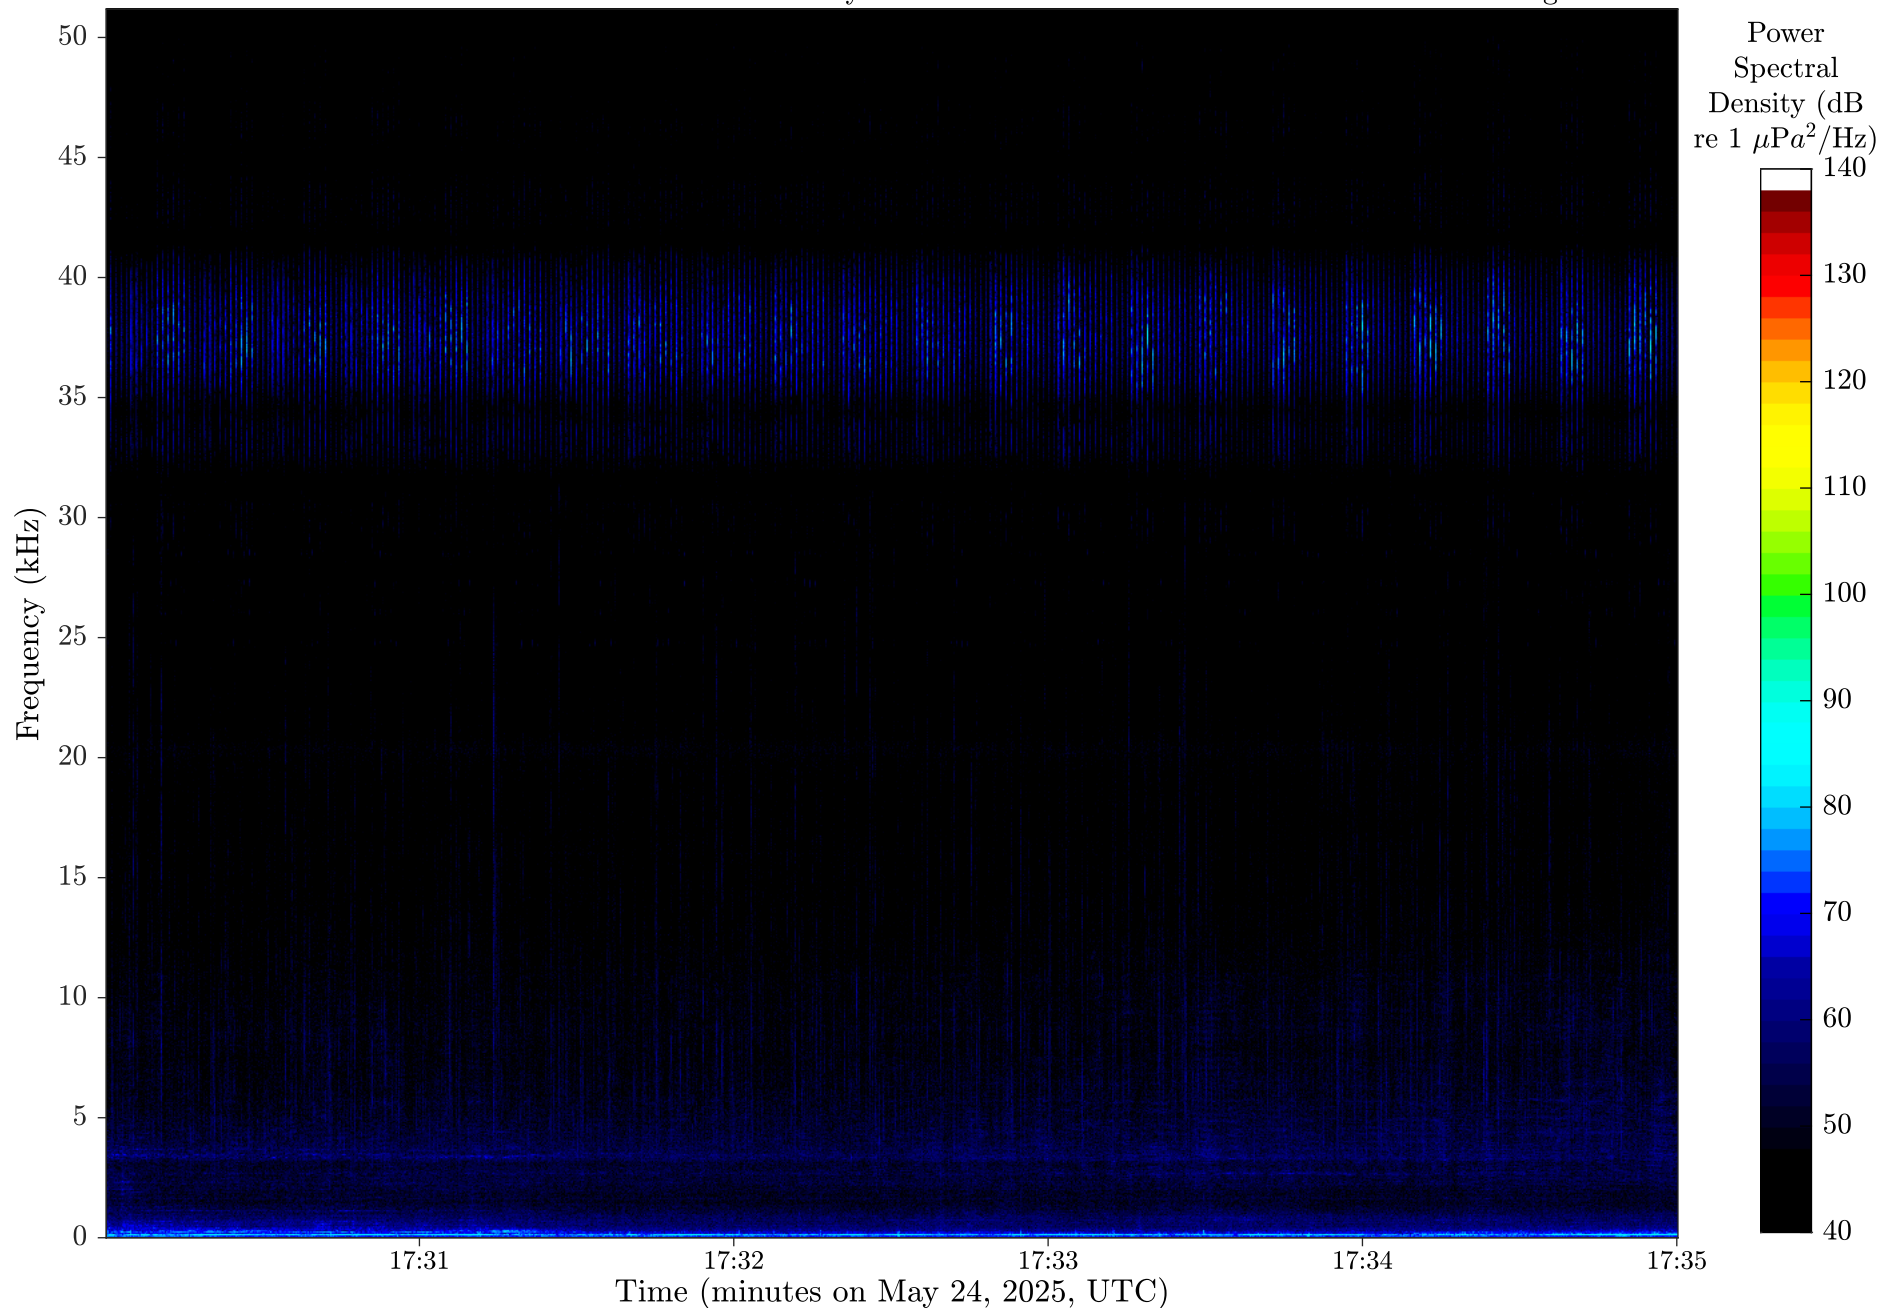


Comments: 31.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:46 UTC

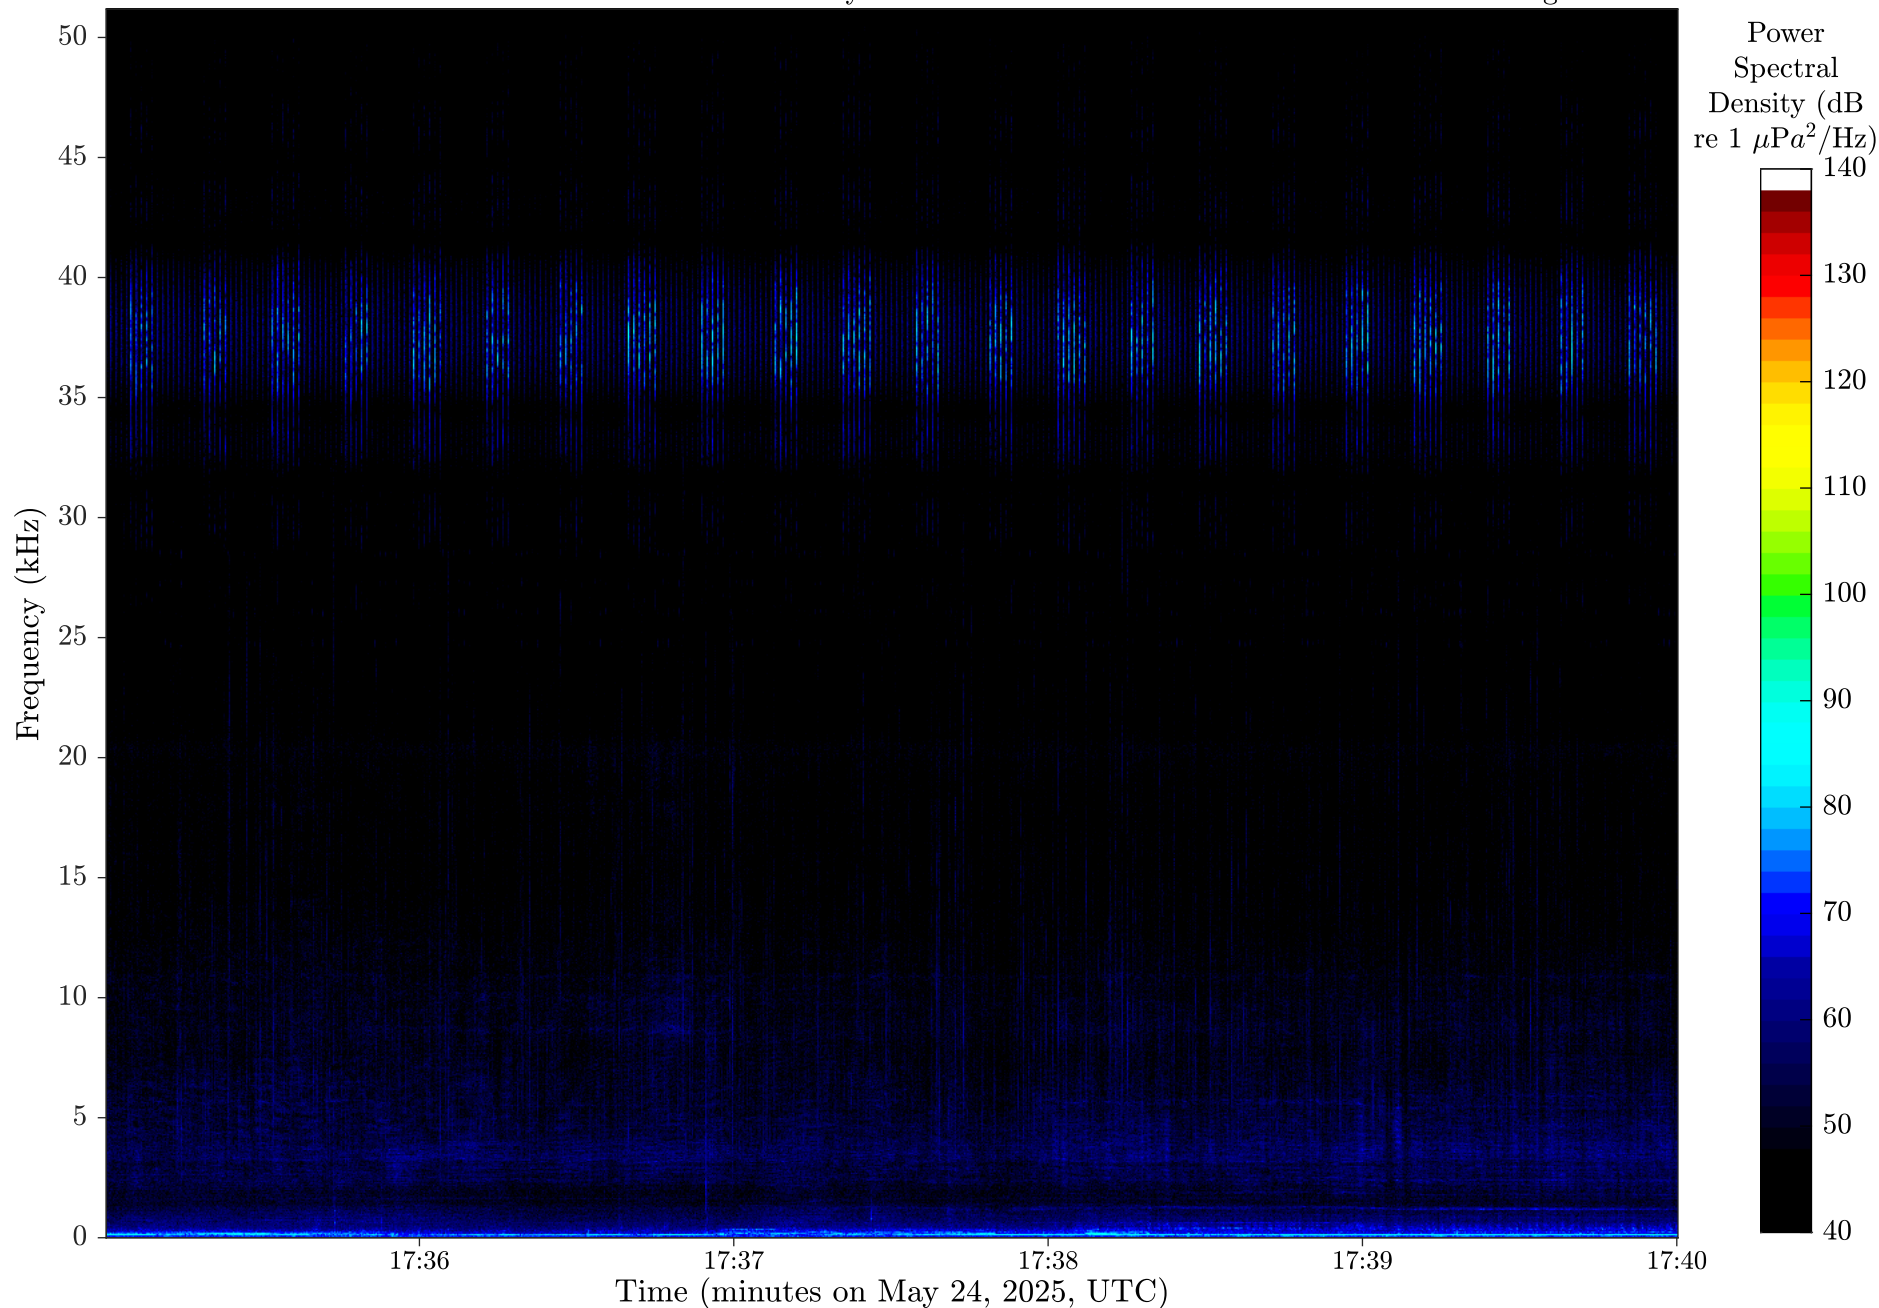


Comments: 30.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:53 UTC

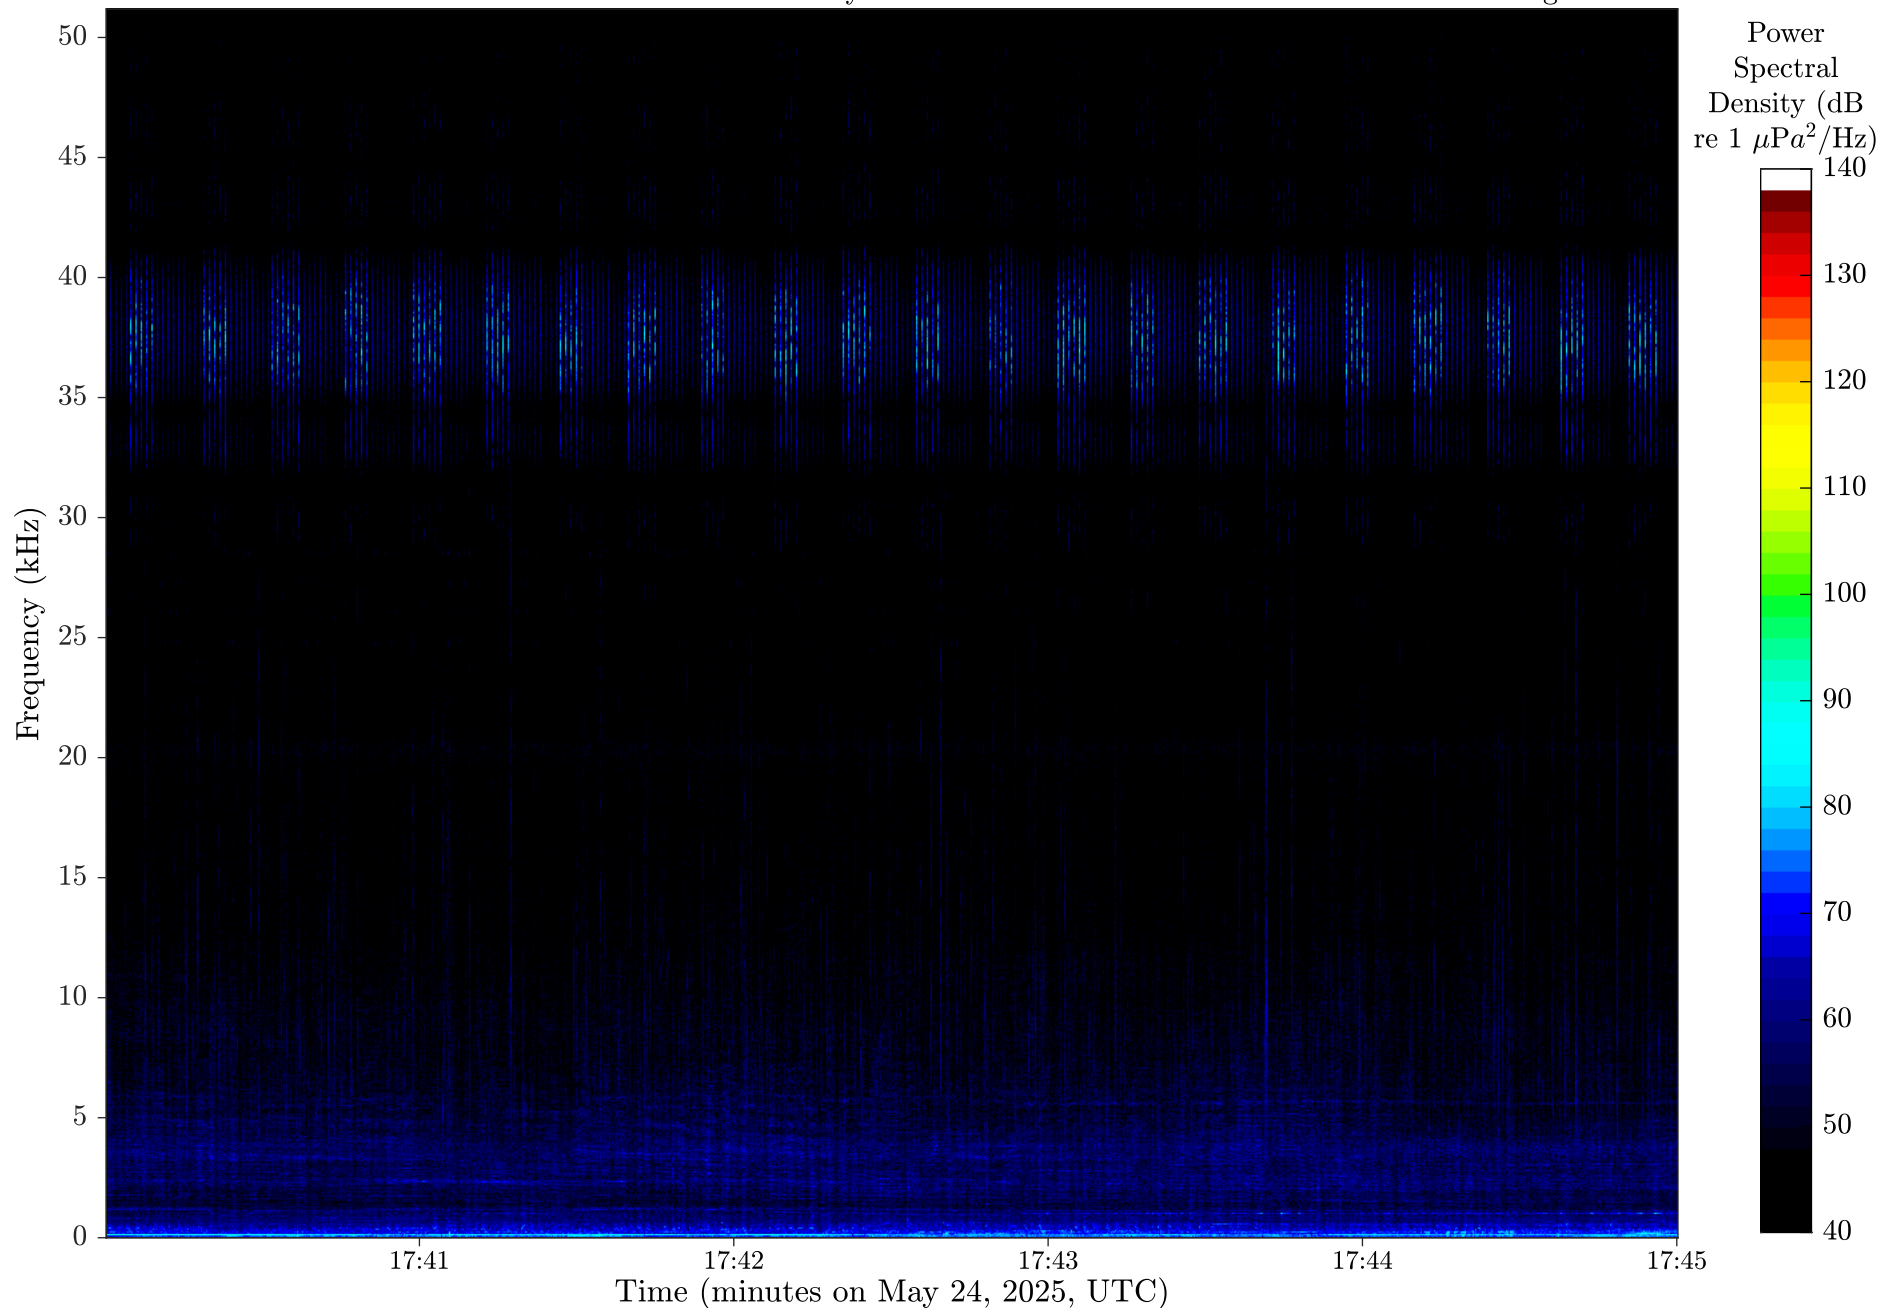


Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:00 UTC

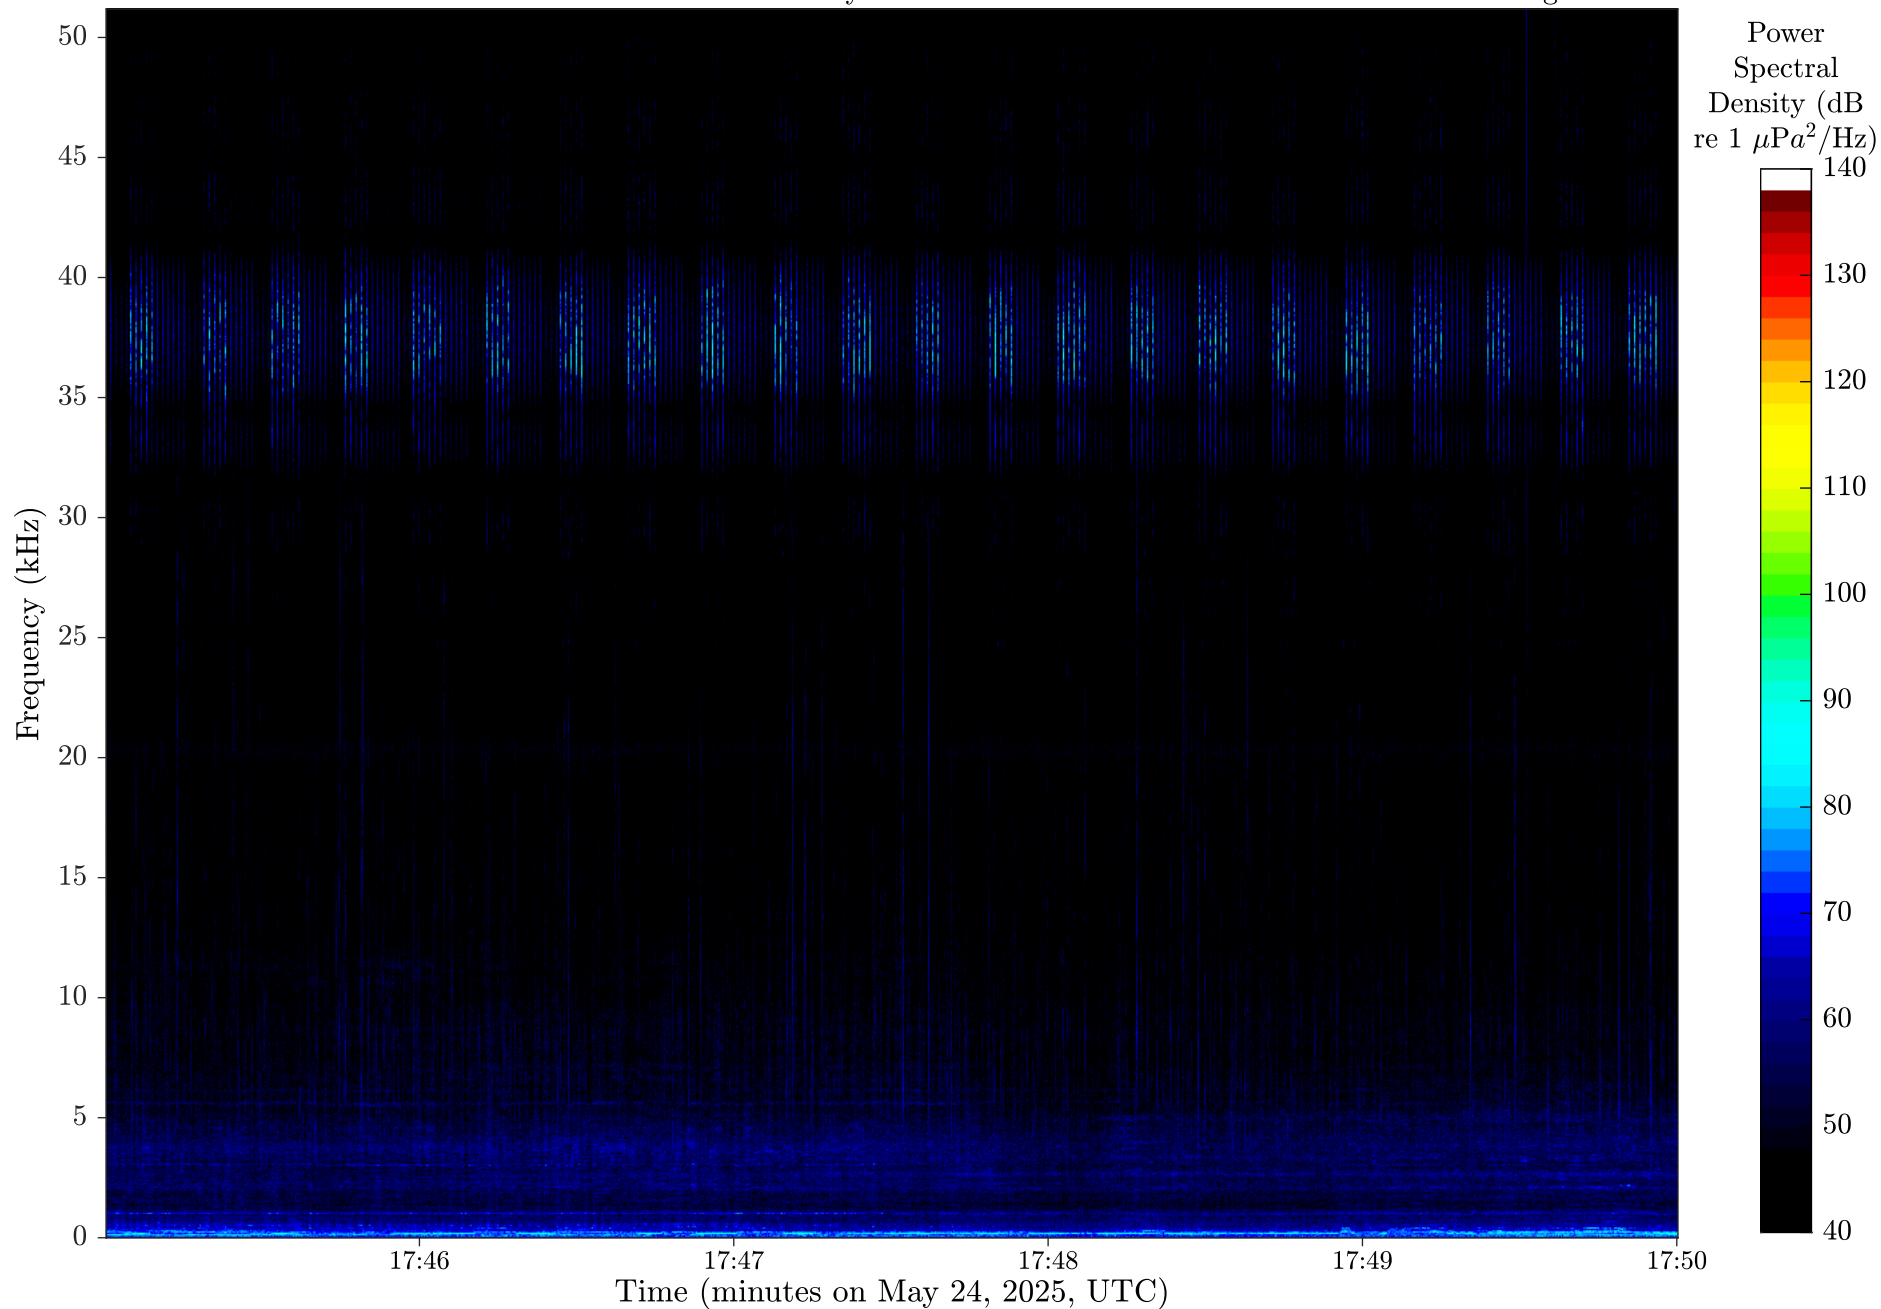


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:08 UTC

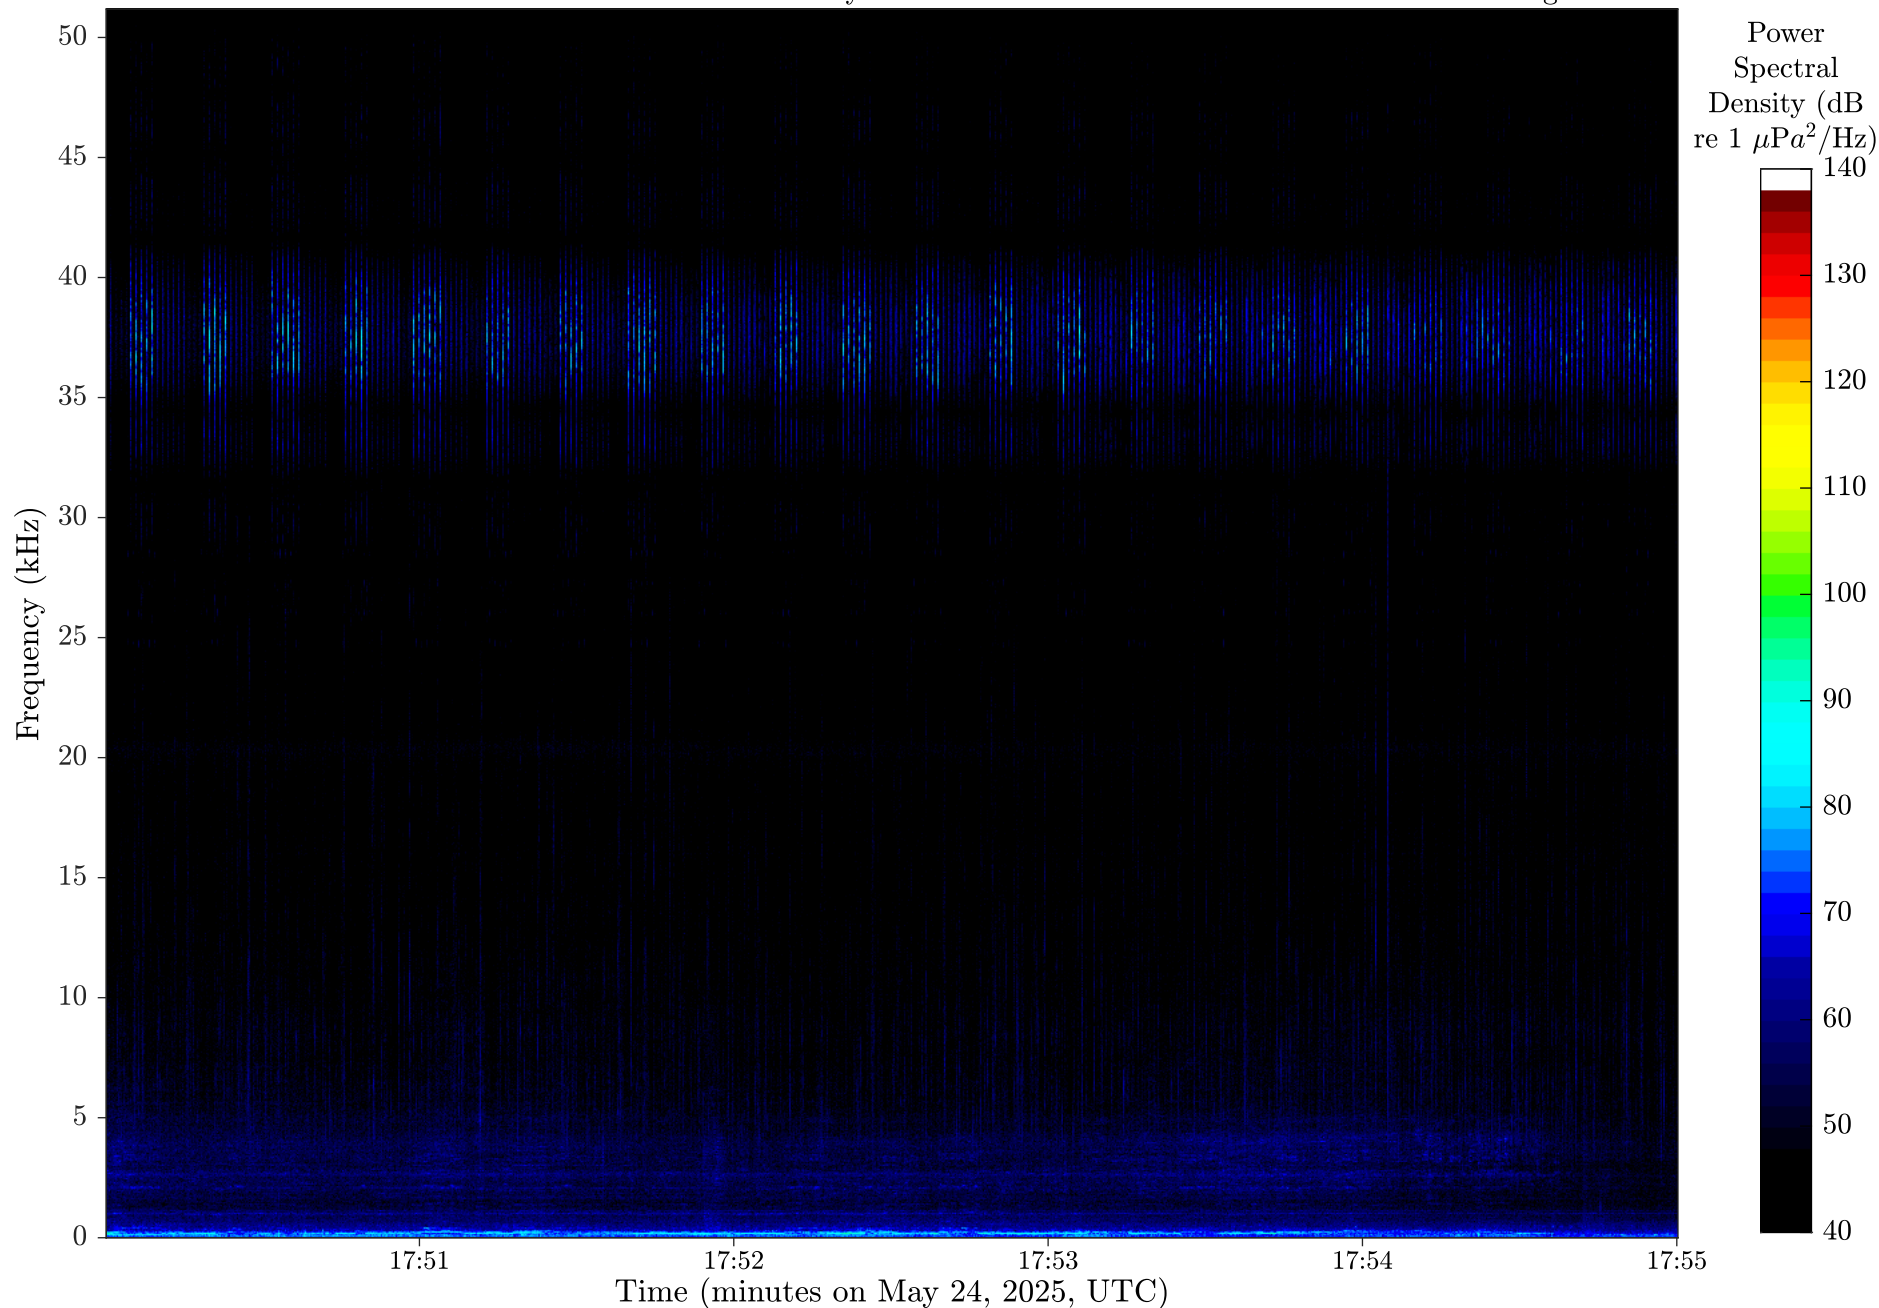


Comments: 32.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:38:15 UTC

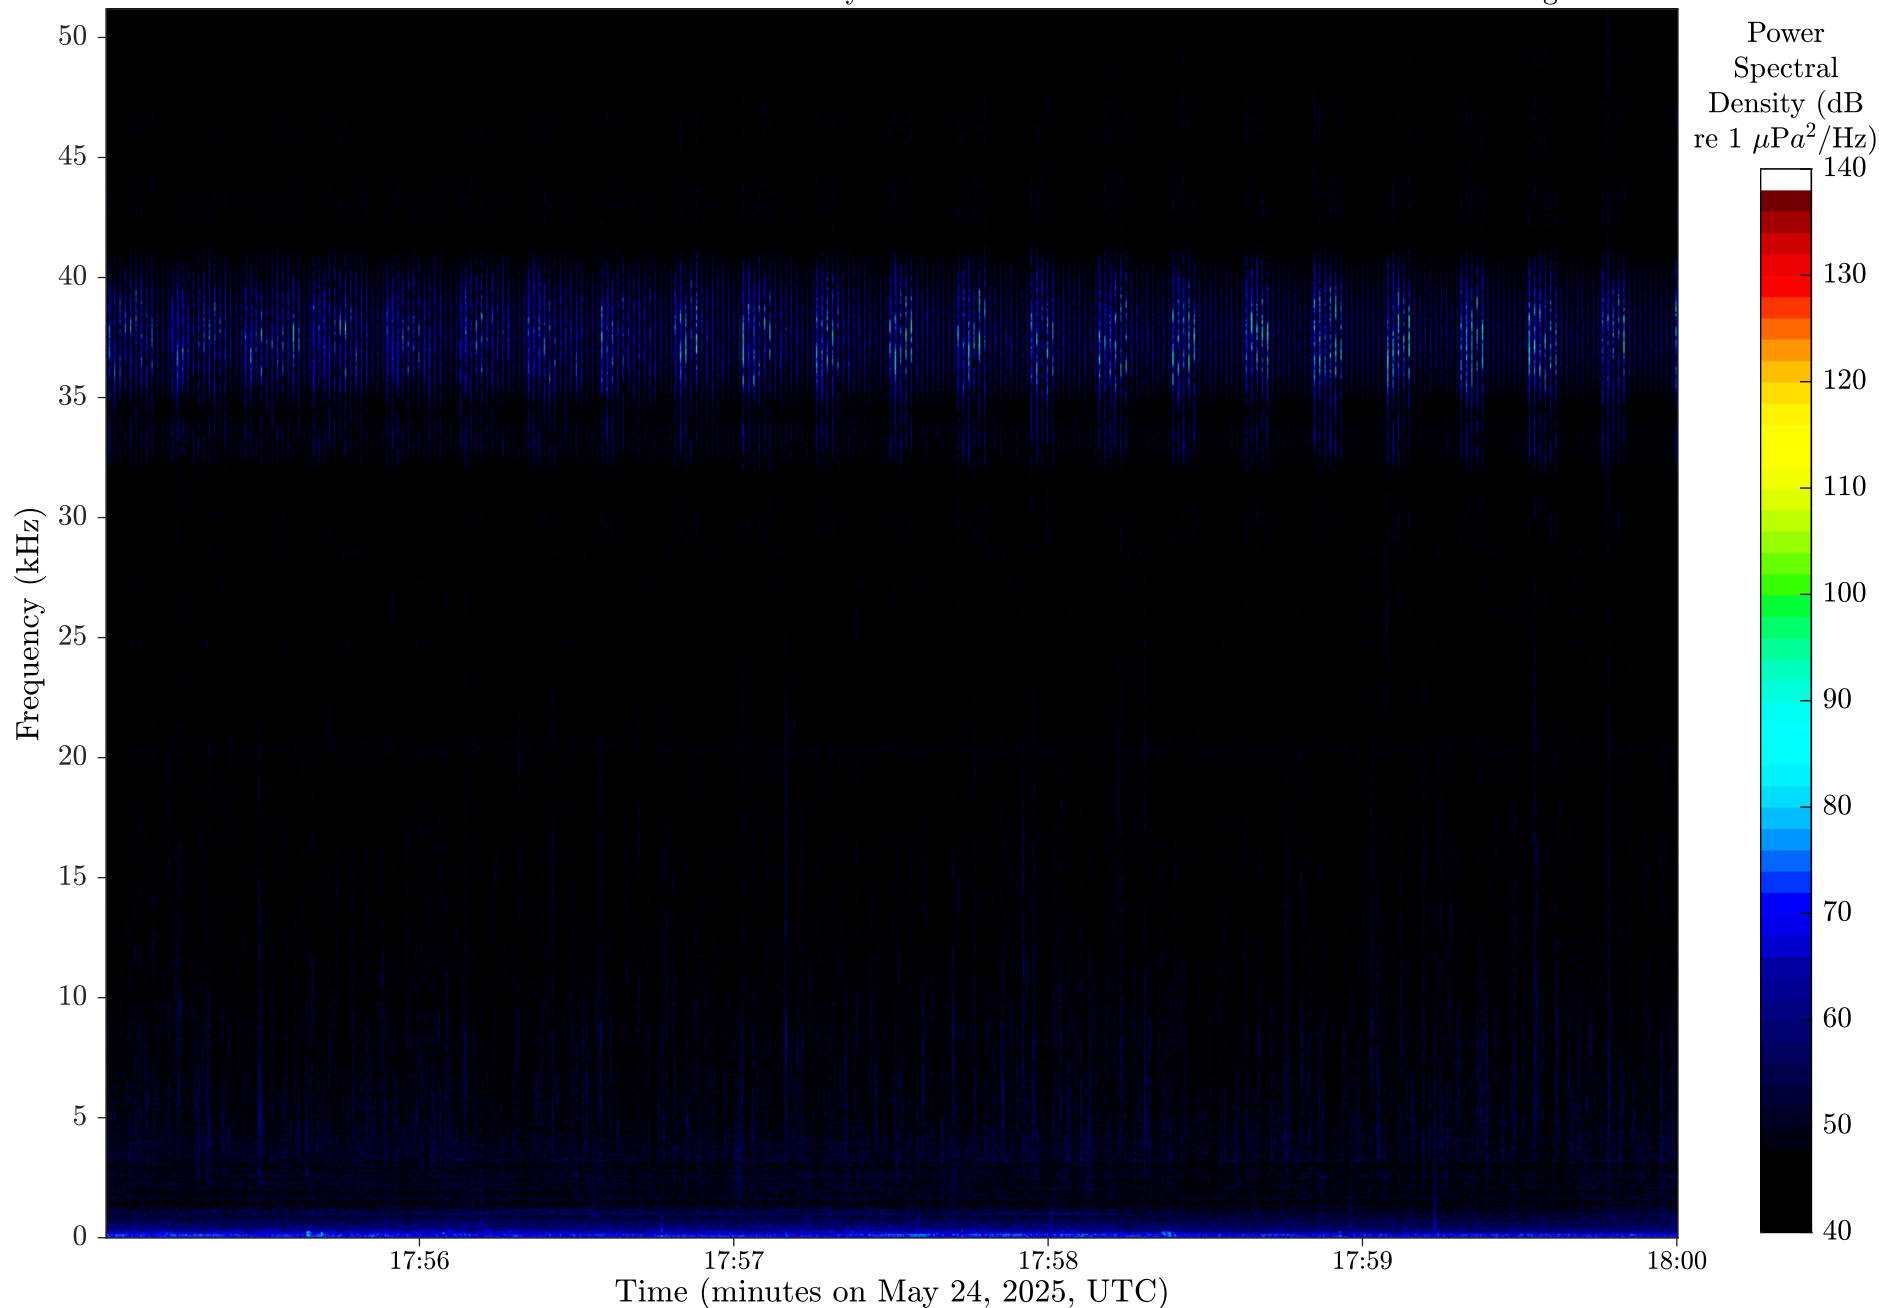

Comments: 32.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:38:22 UTC

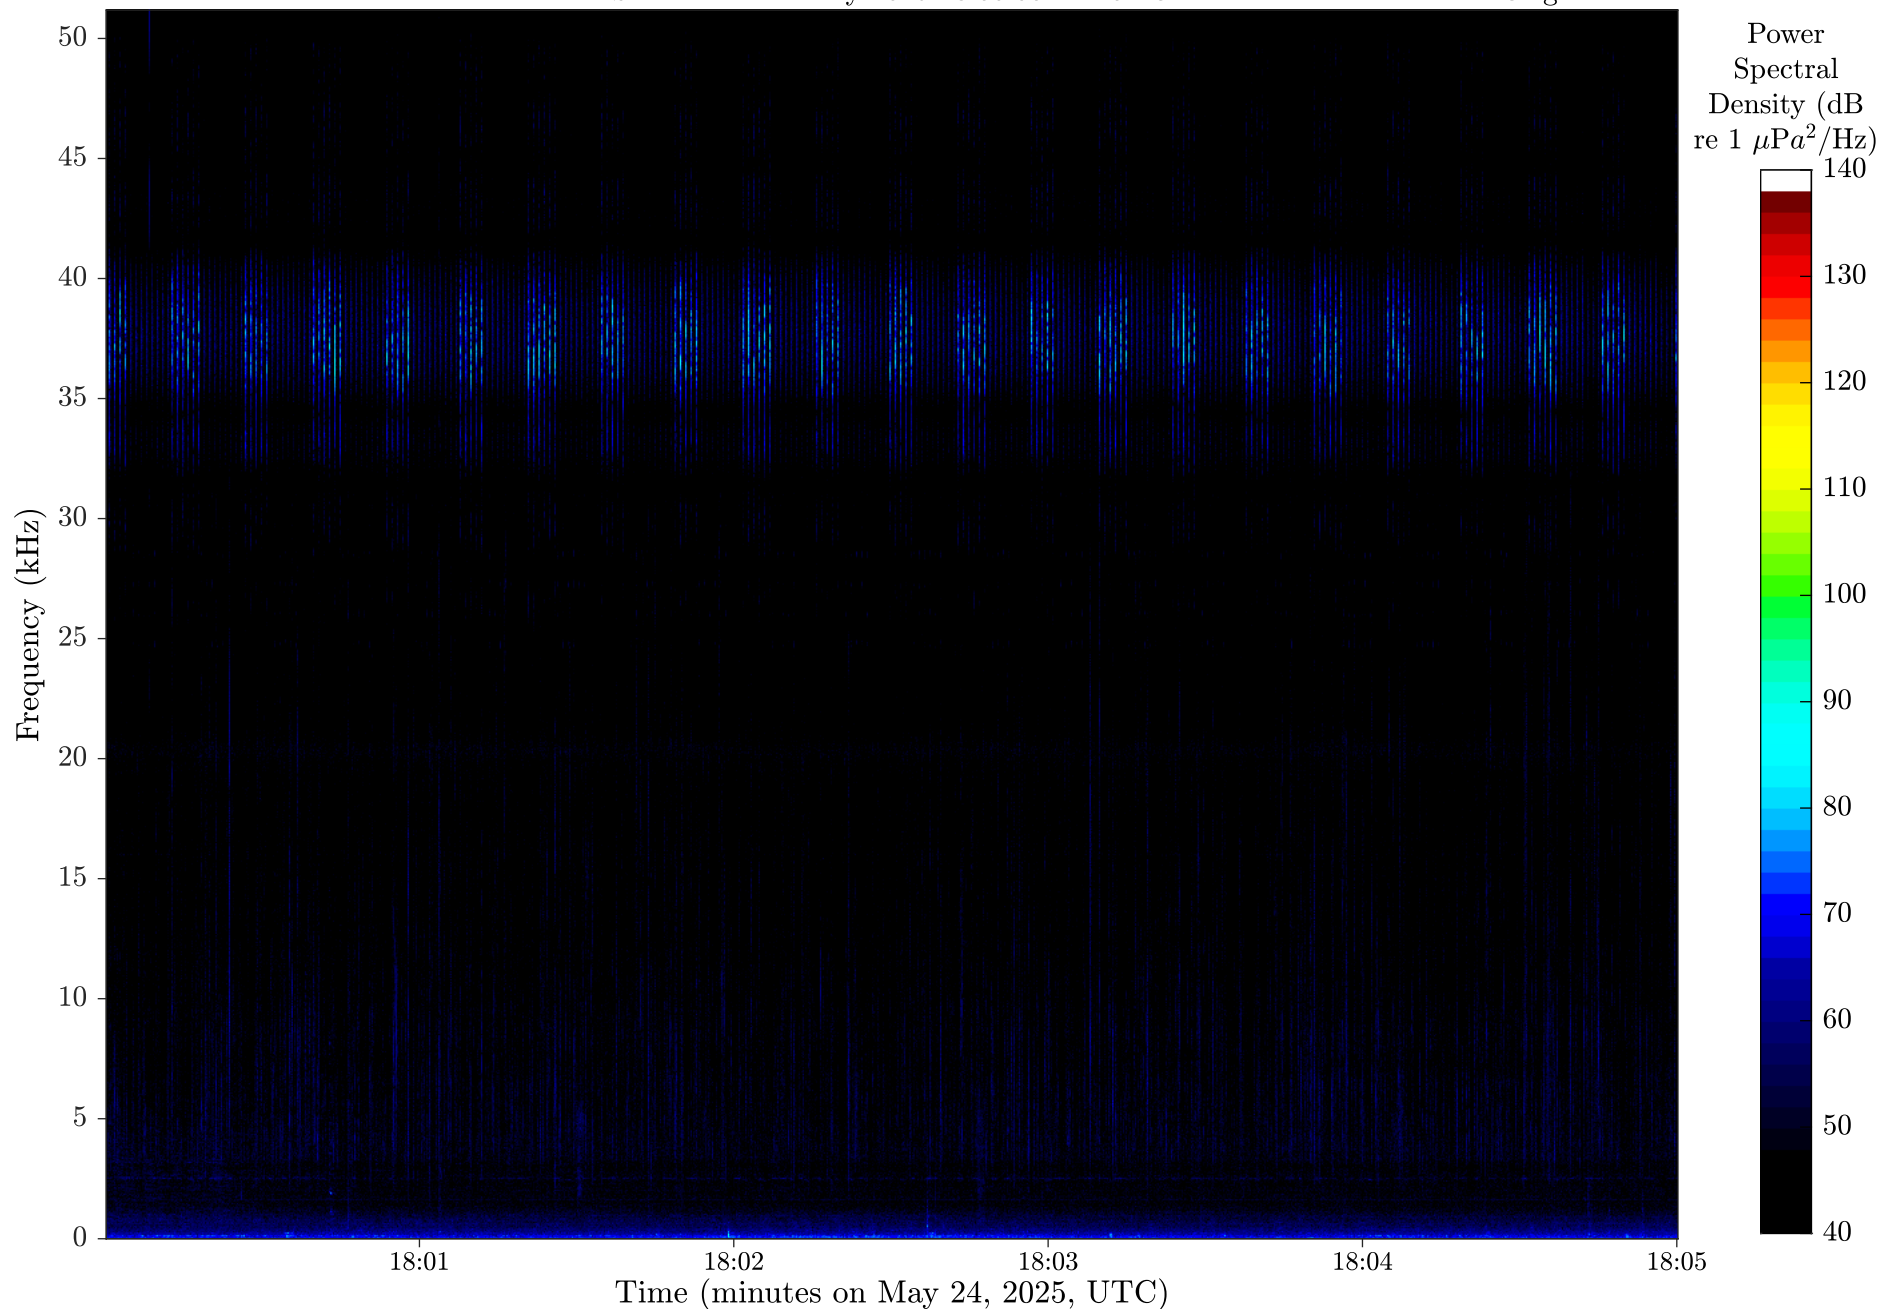

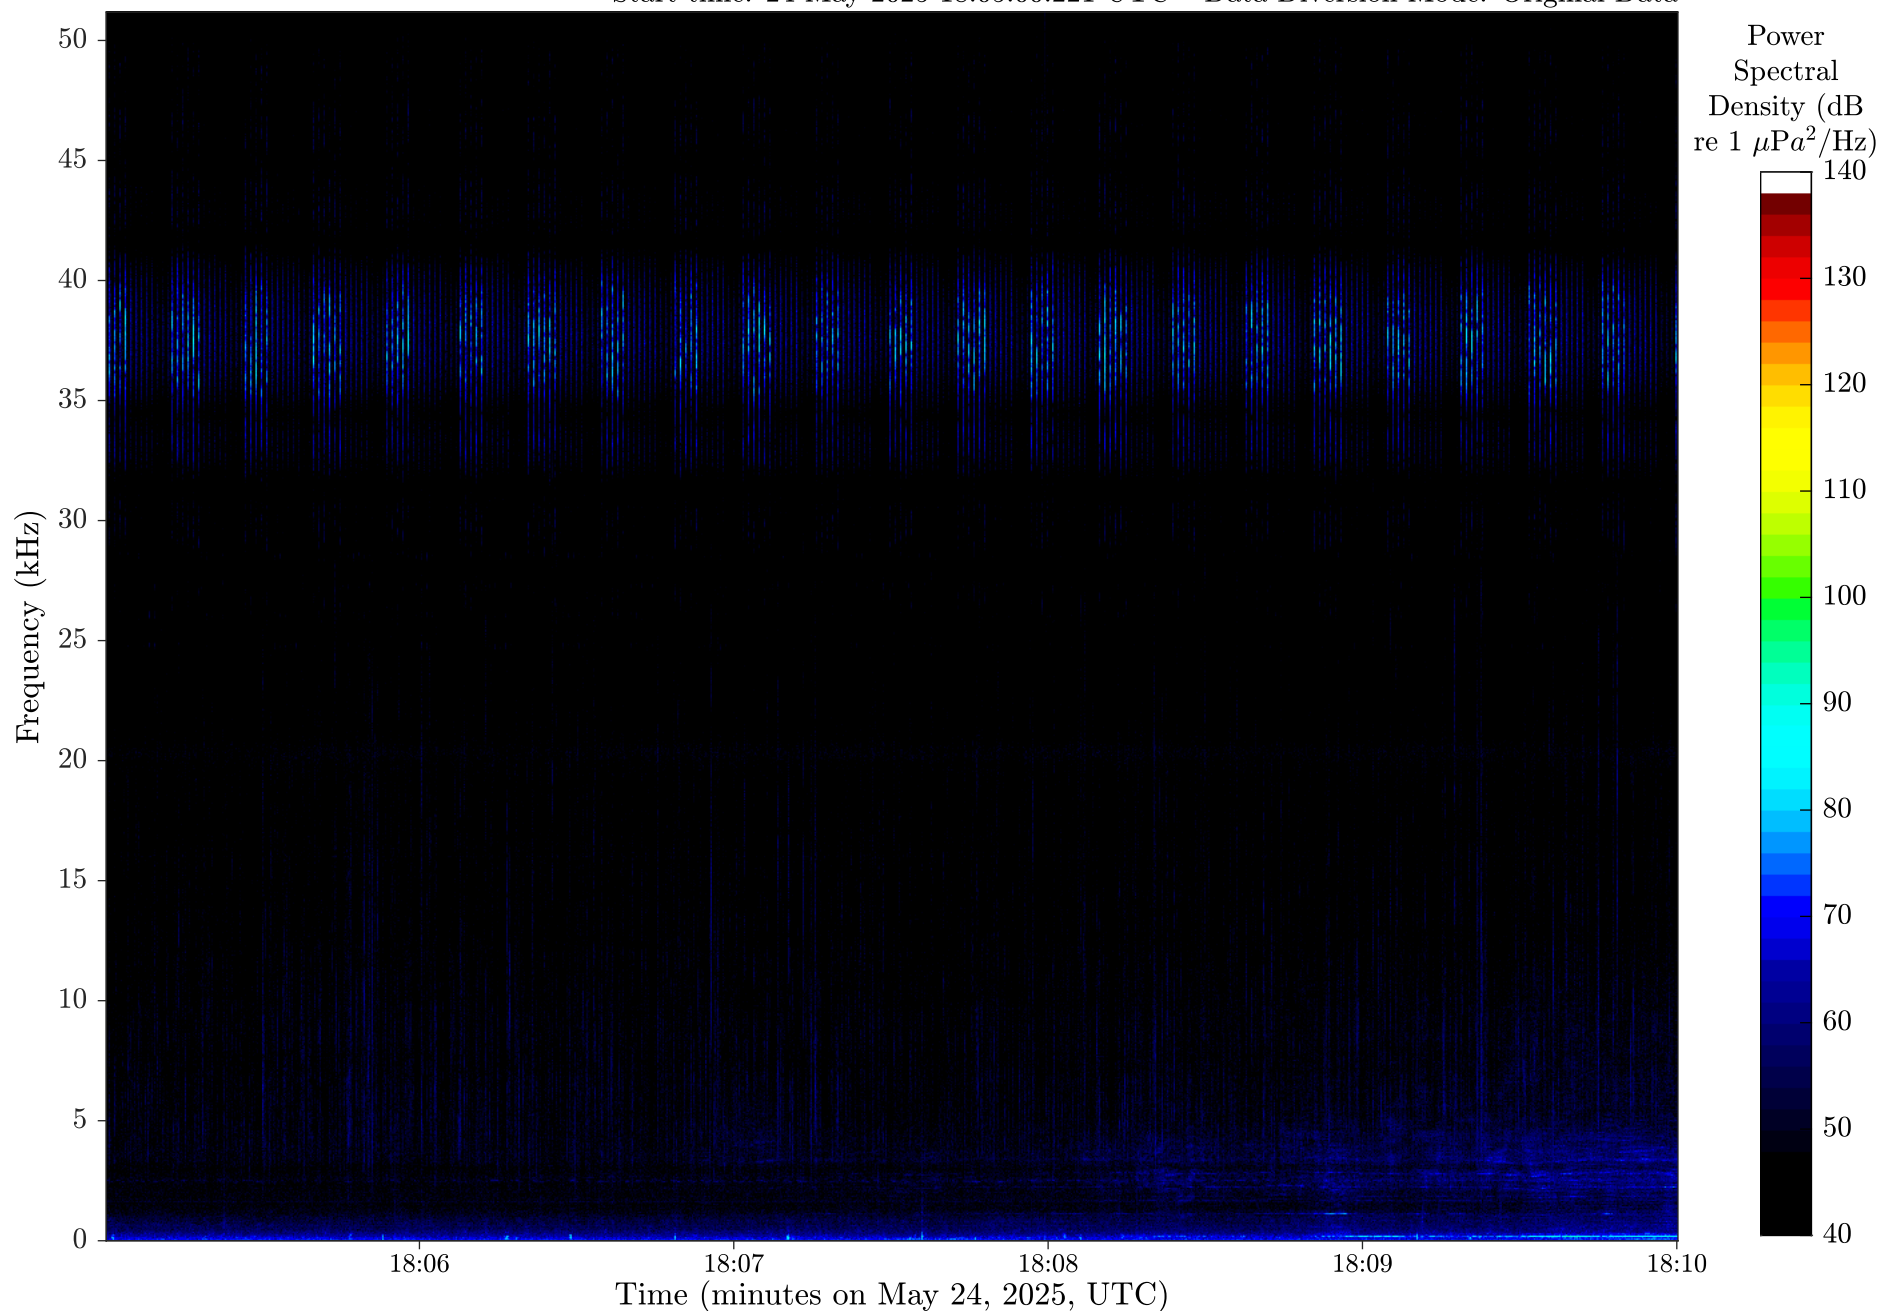


Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:37 UTC

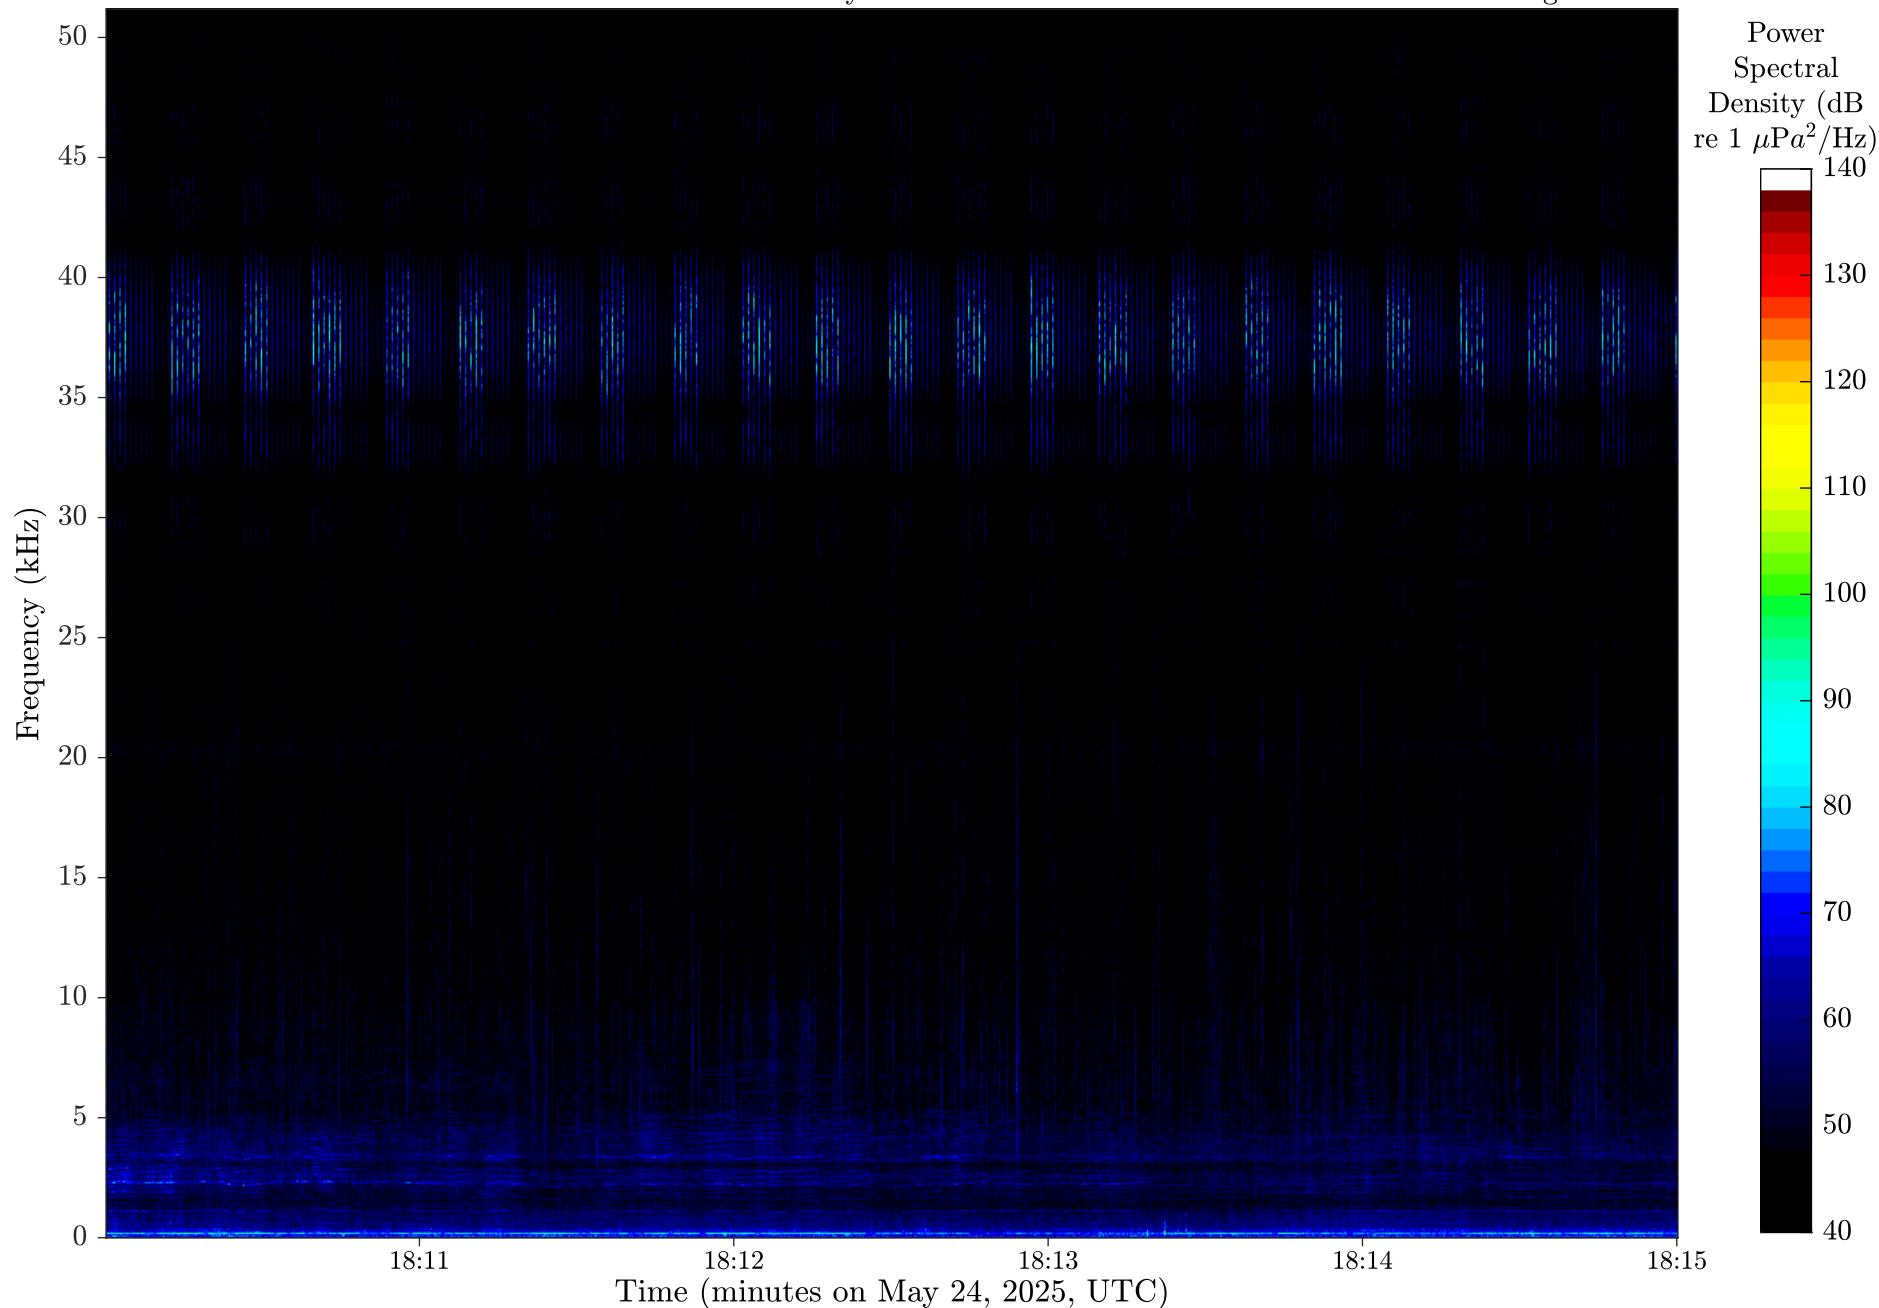


Comments: 32.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:44 UTC

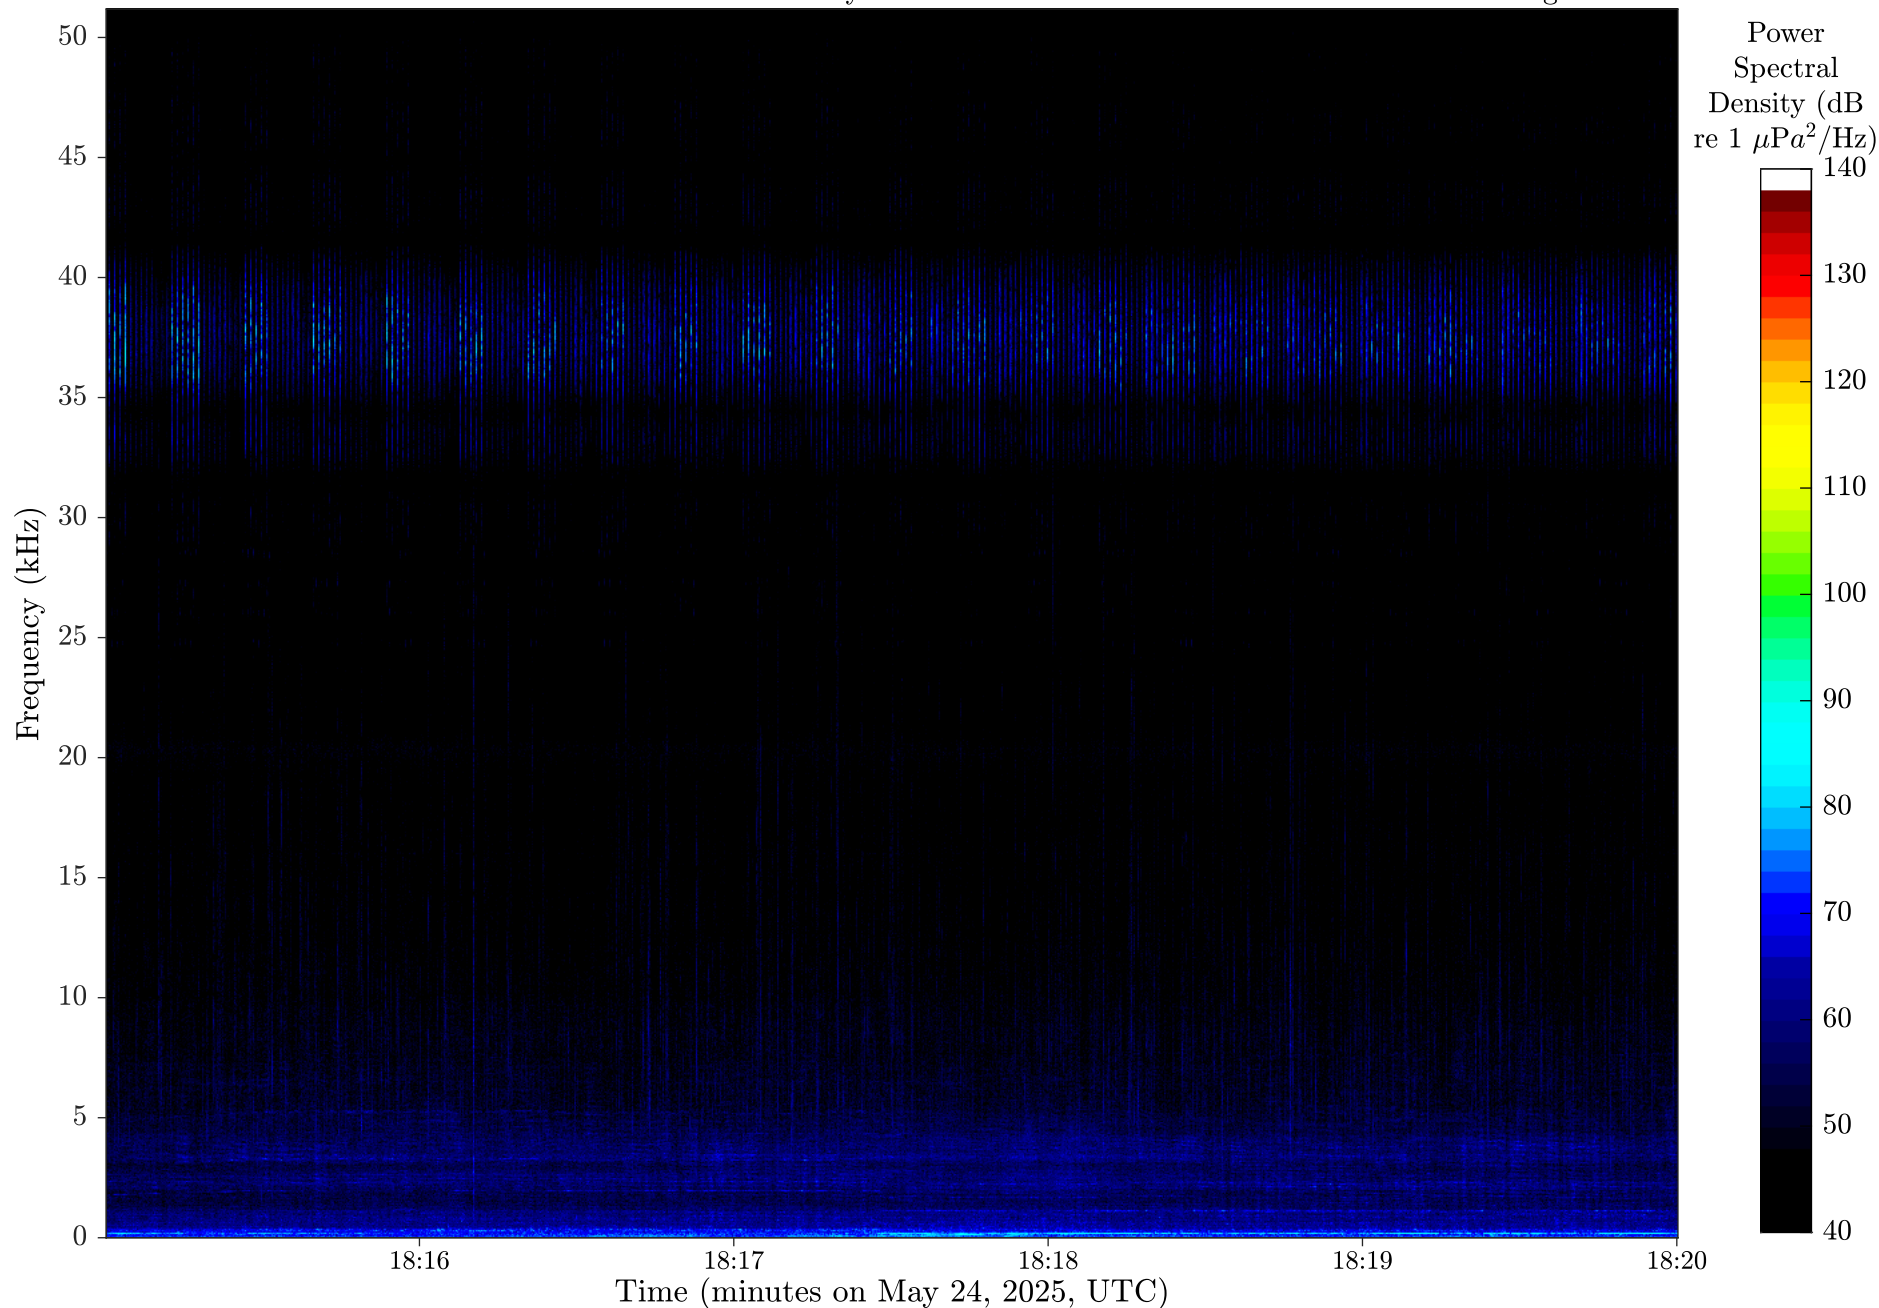


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:51 UTC

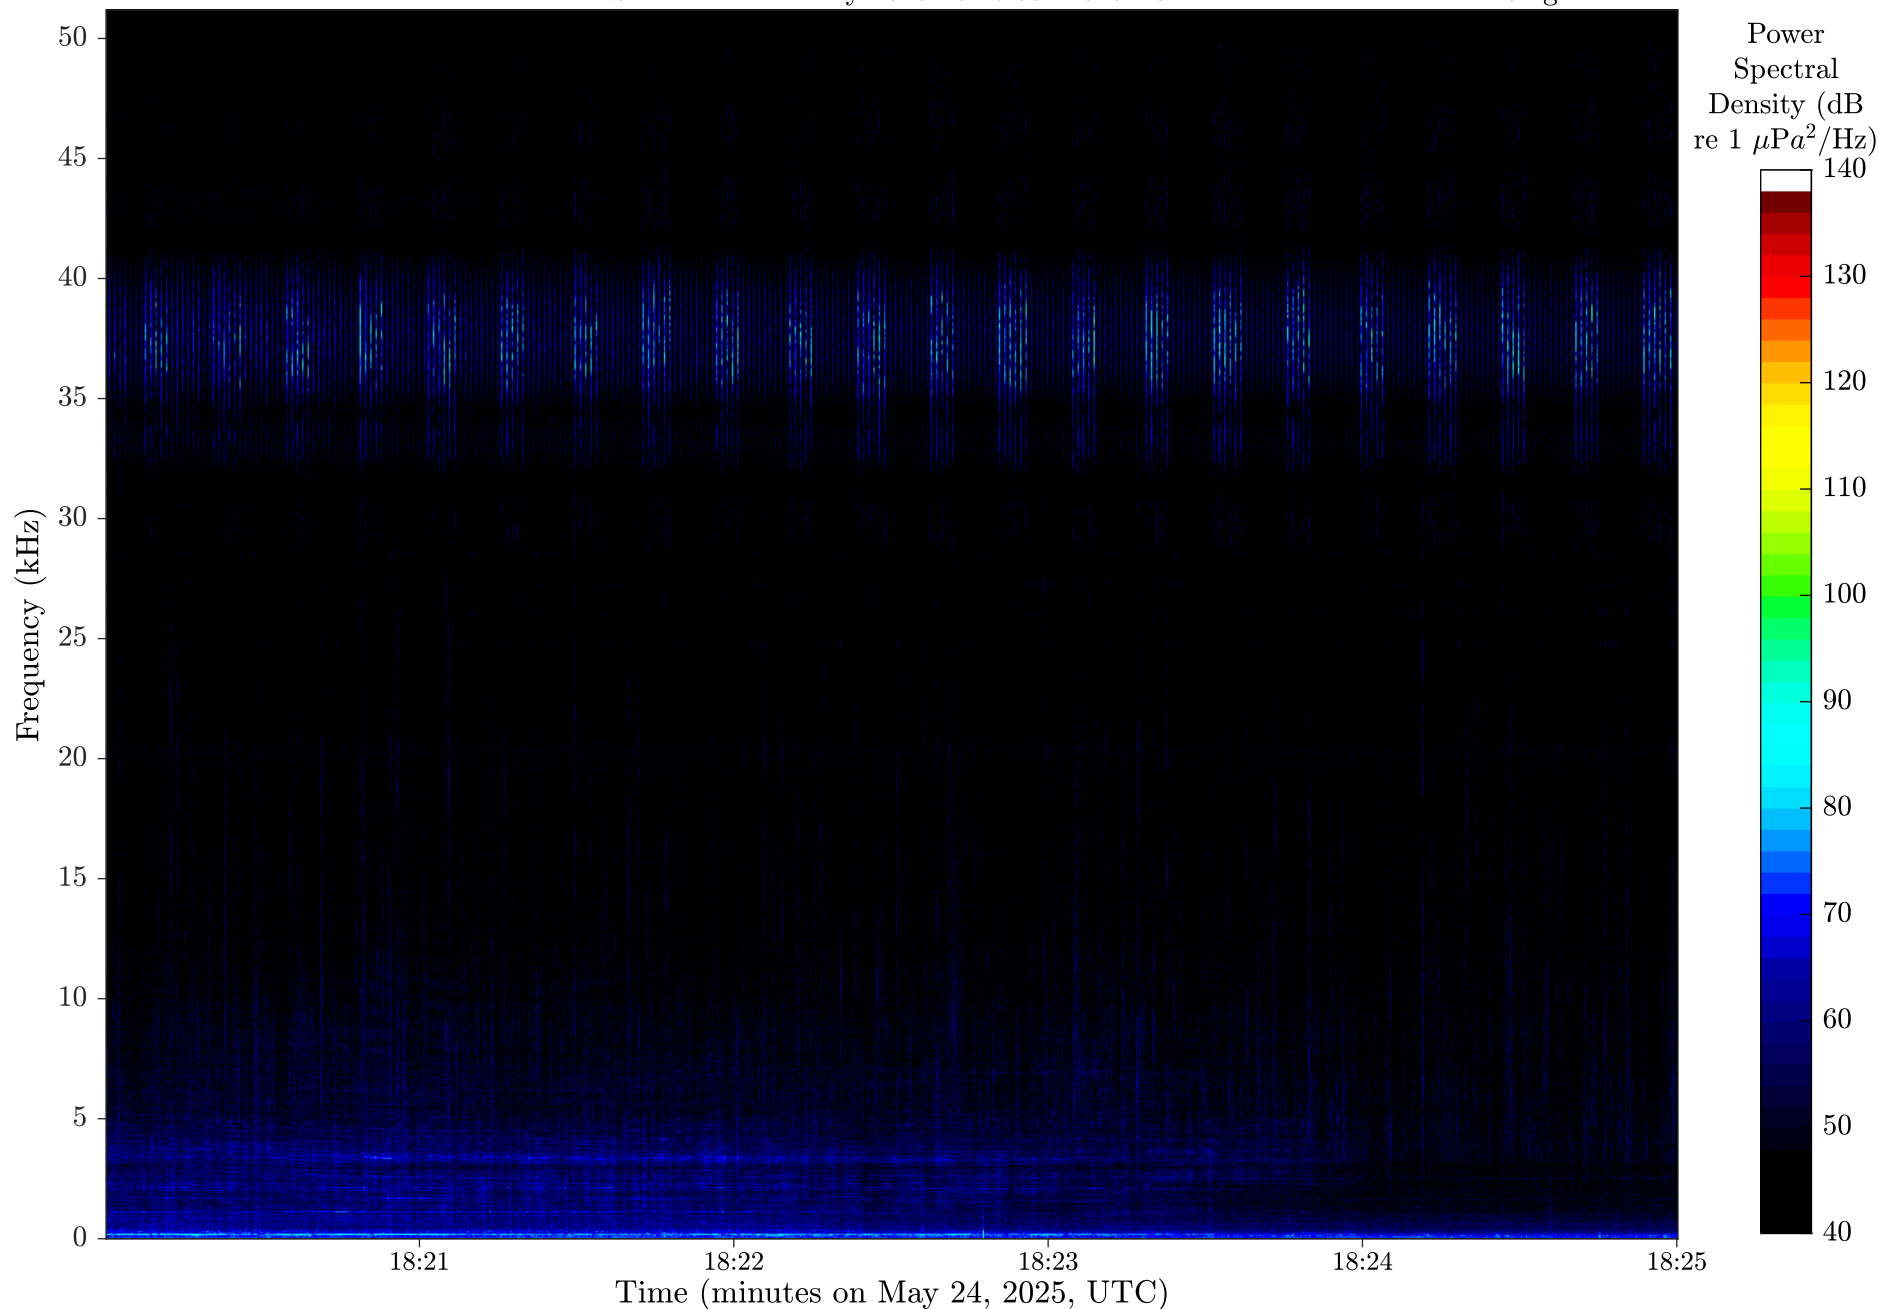


Comments: 31.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:58 UTC

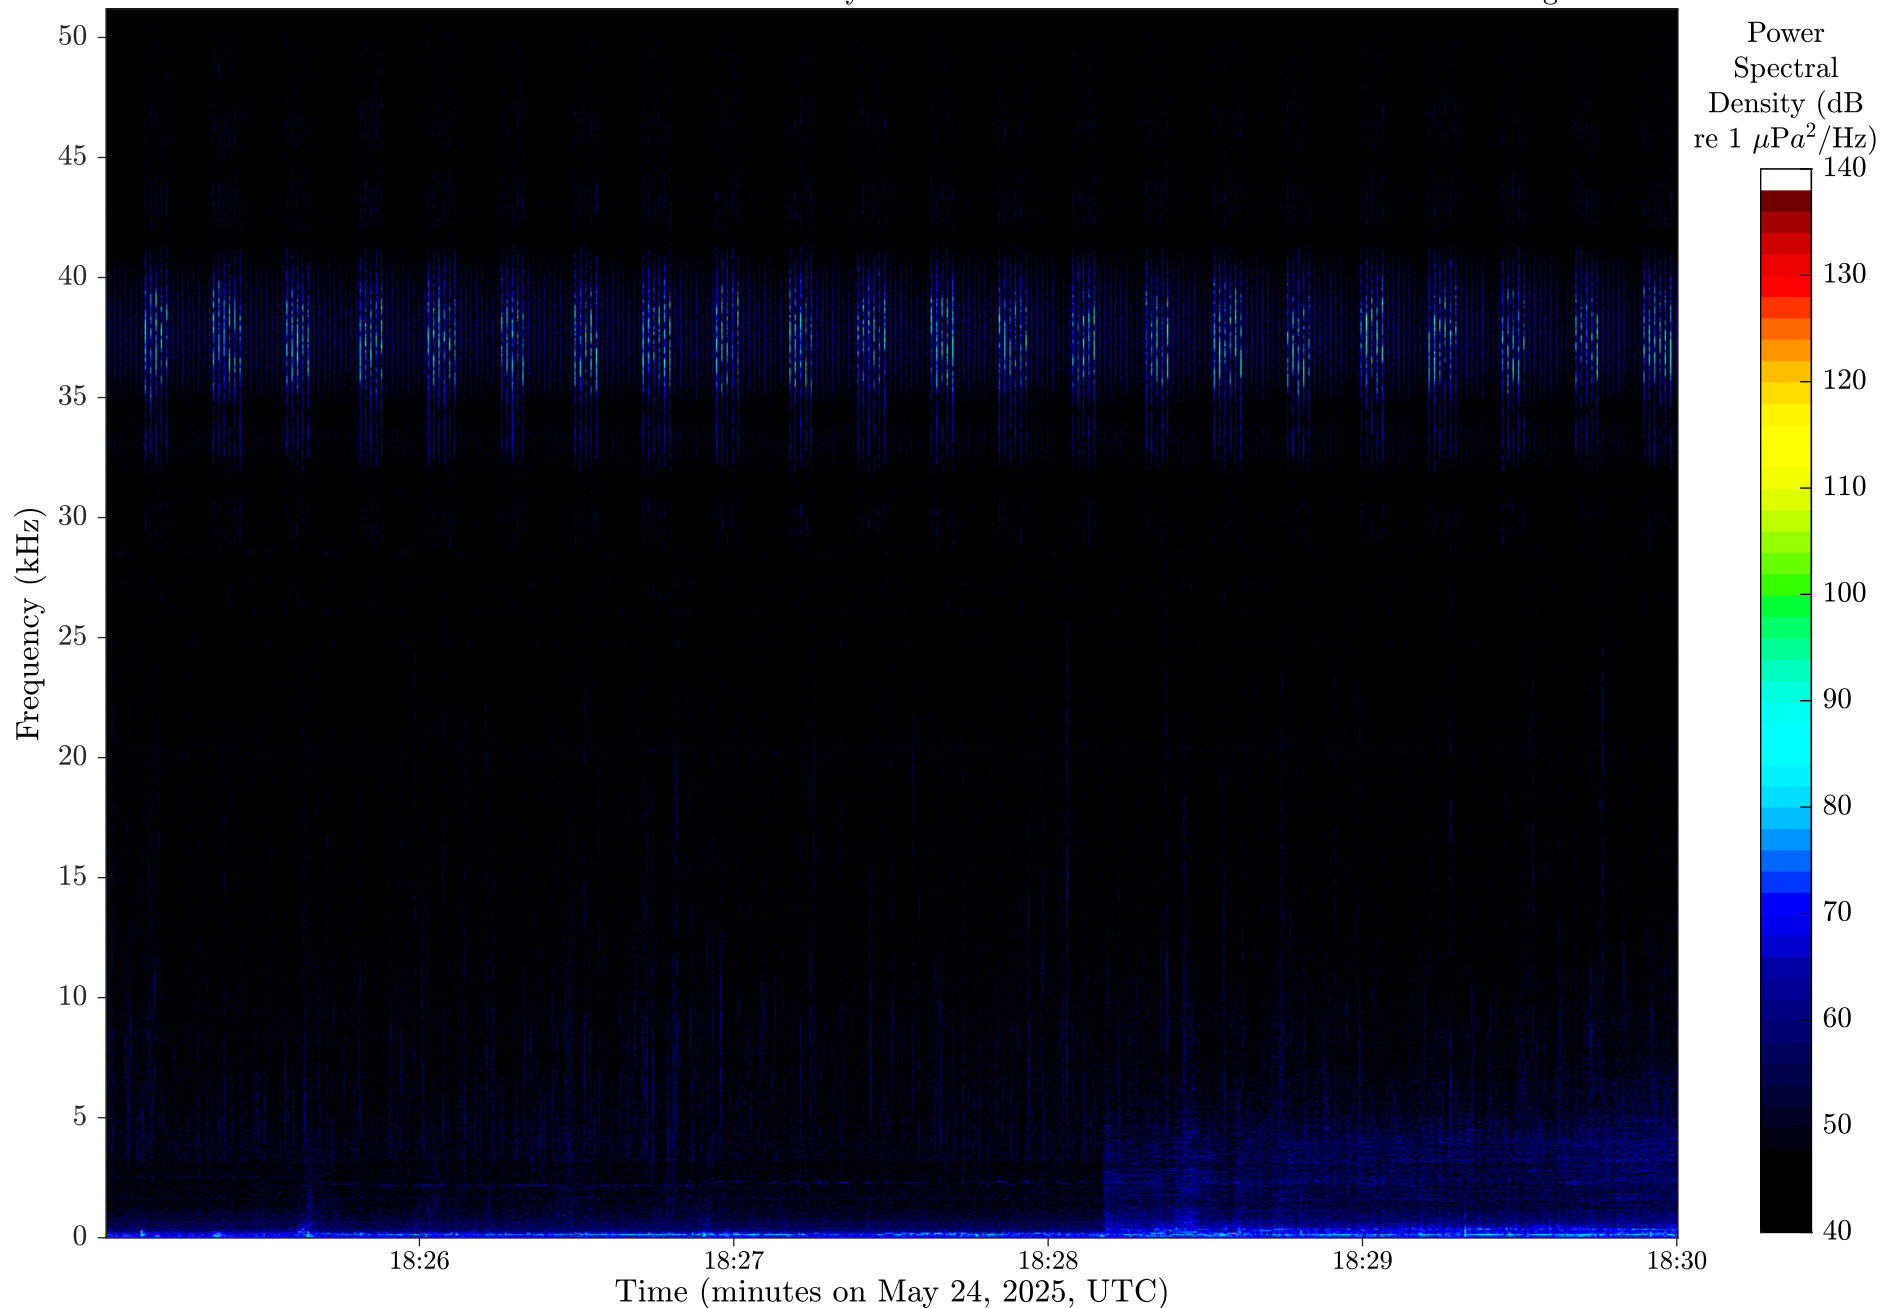


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:05 UTC

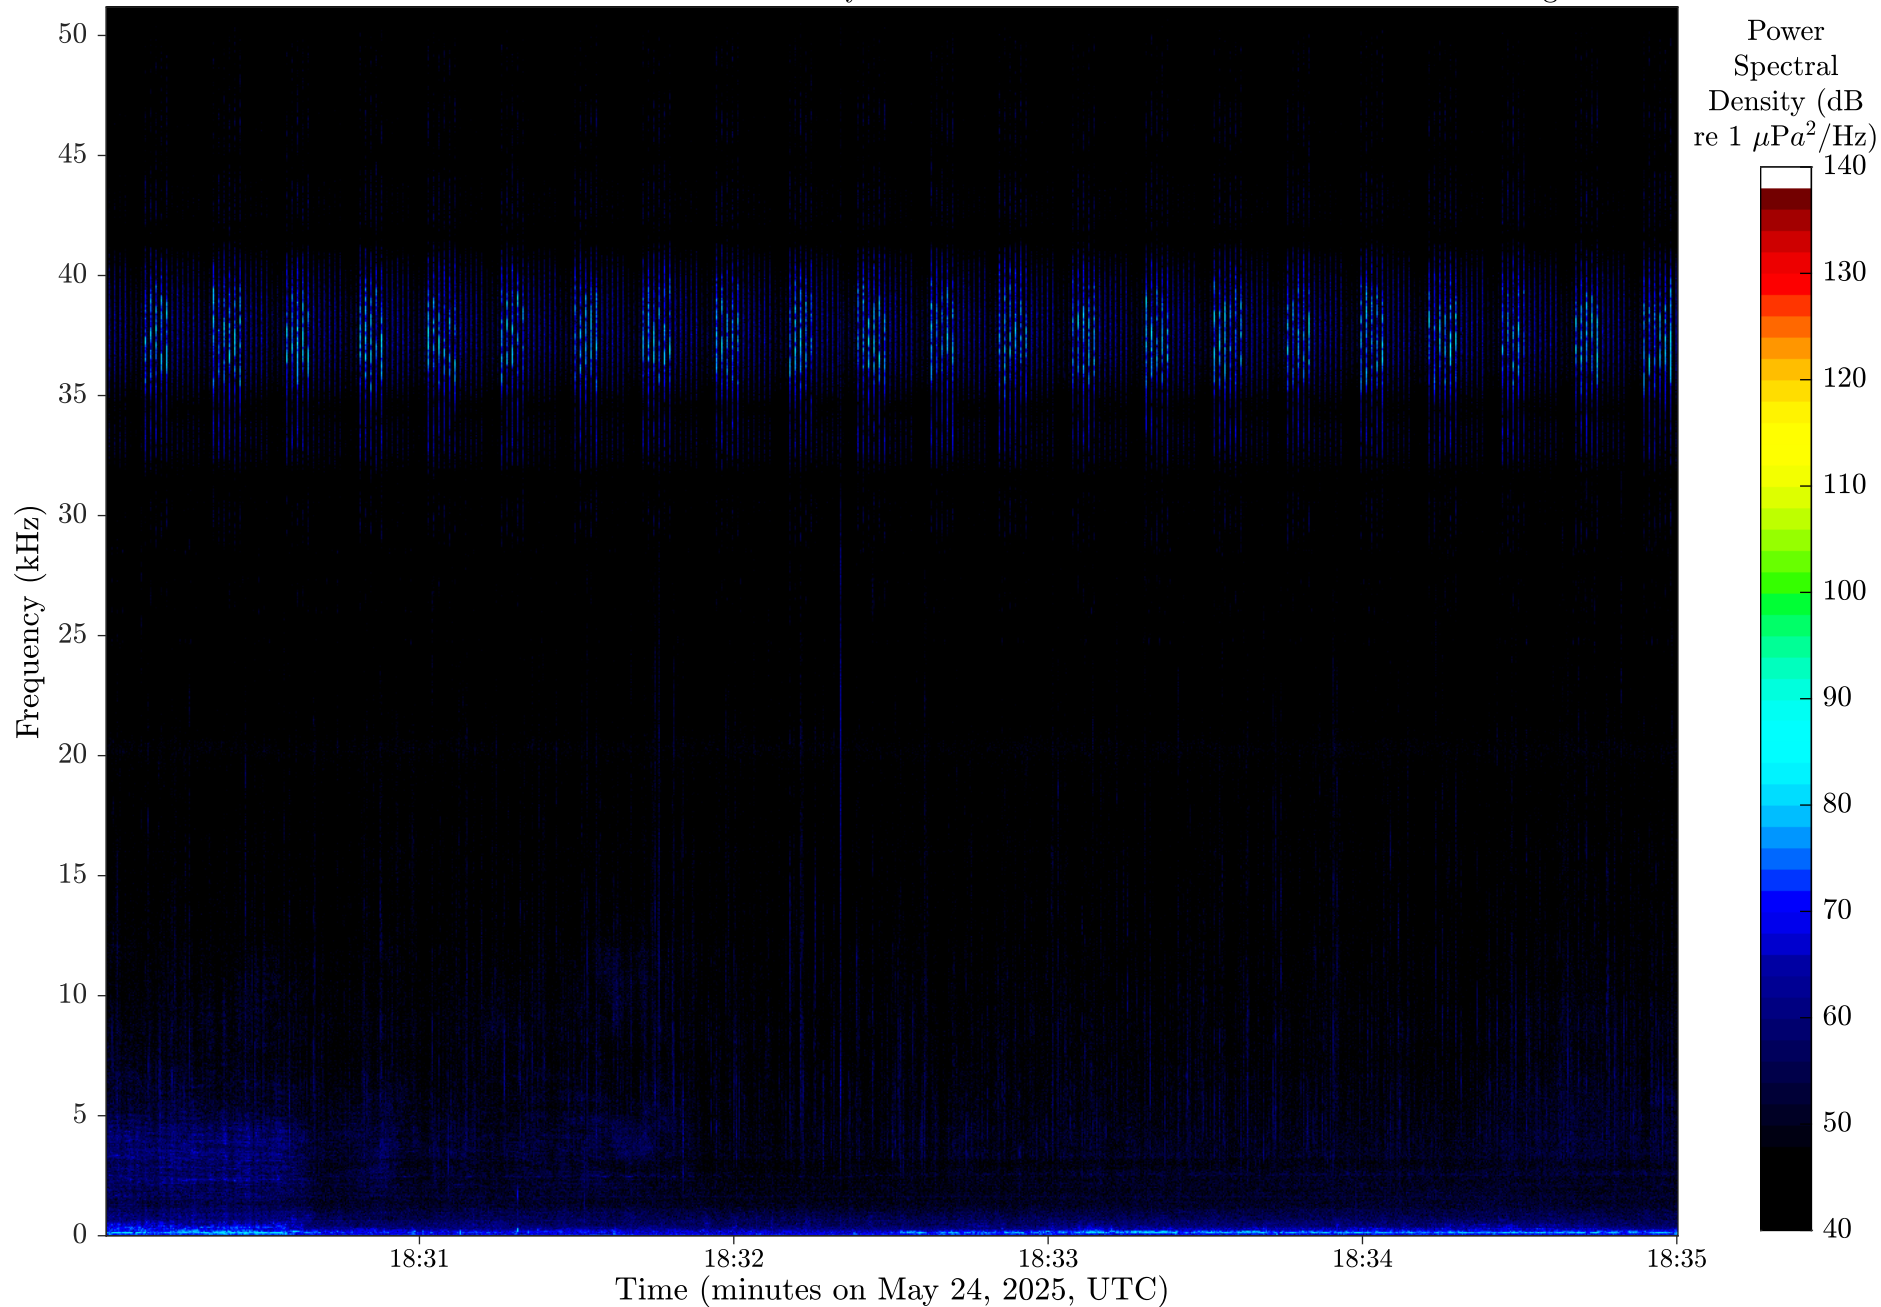


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:13 UTC

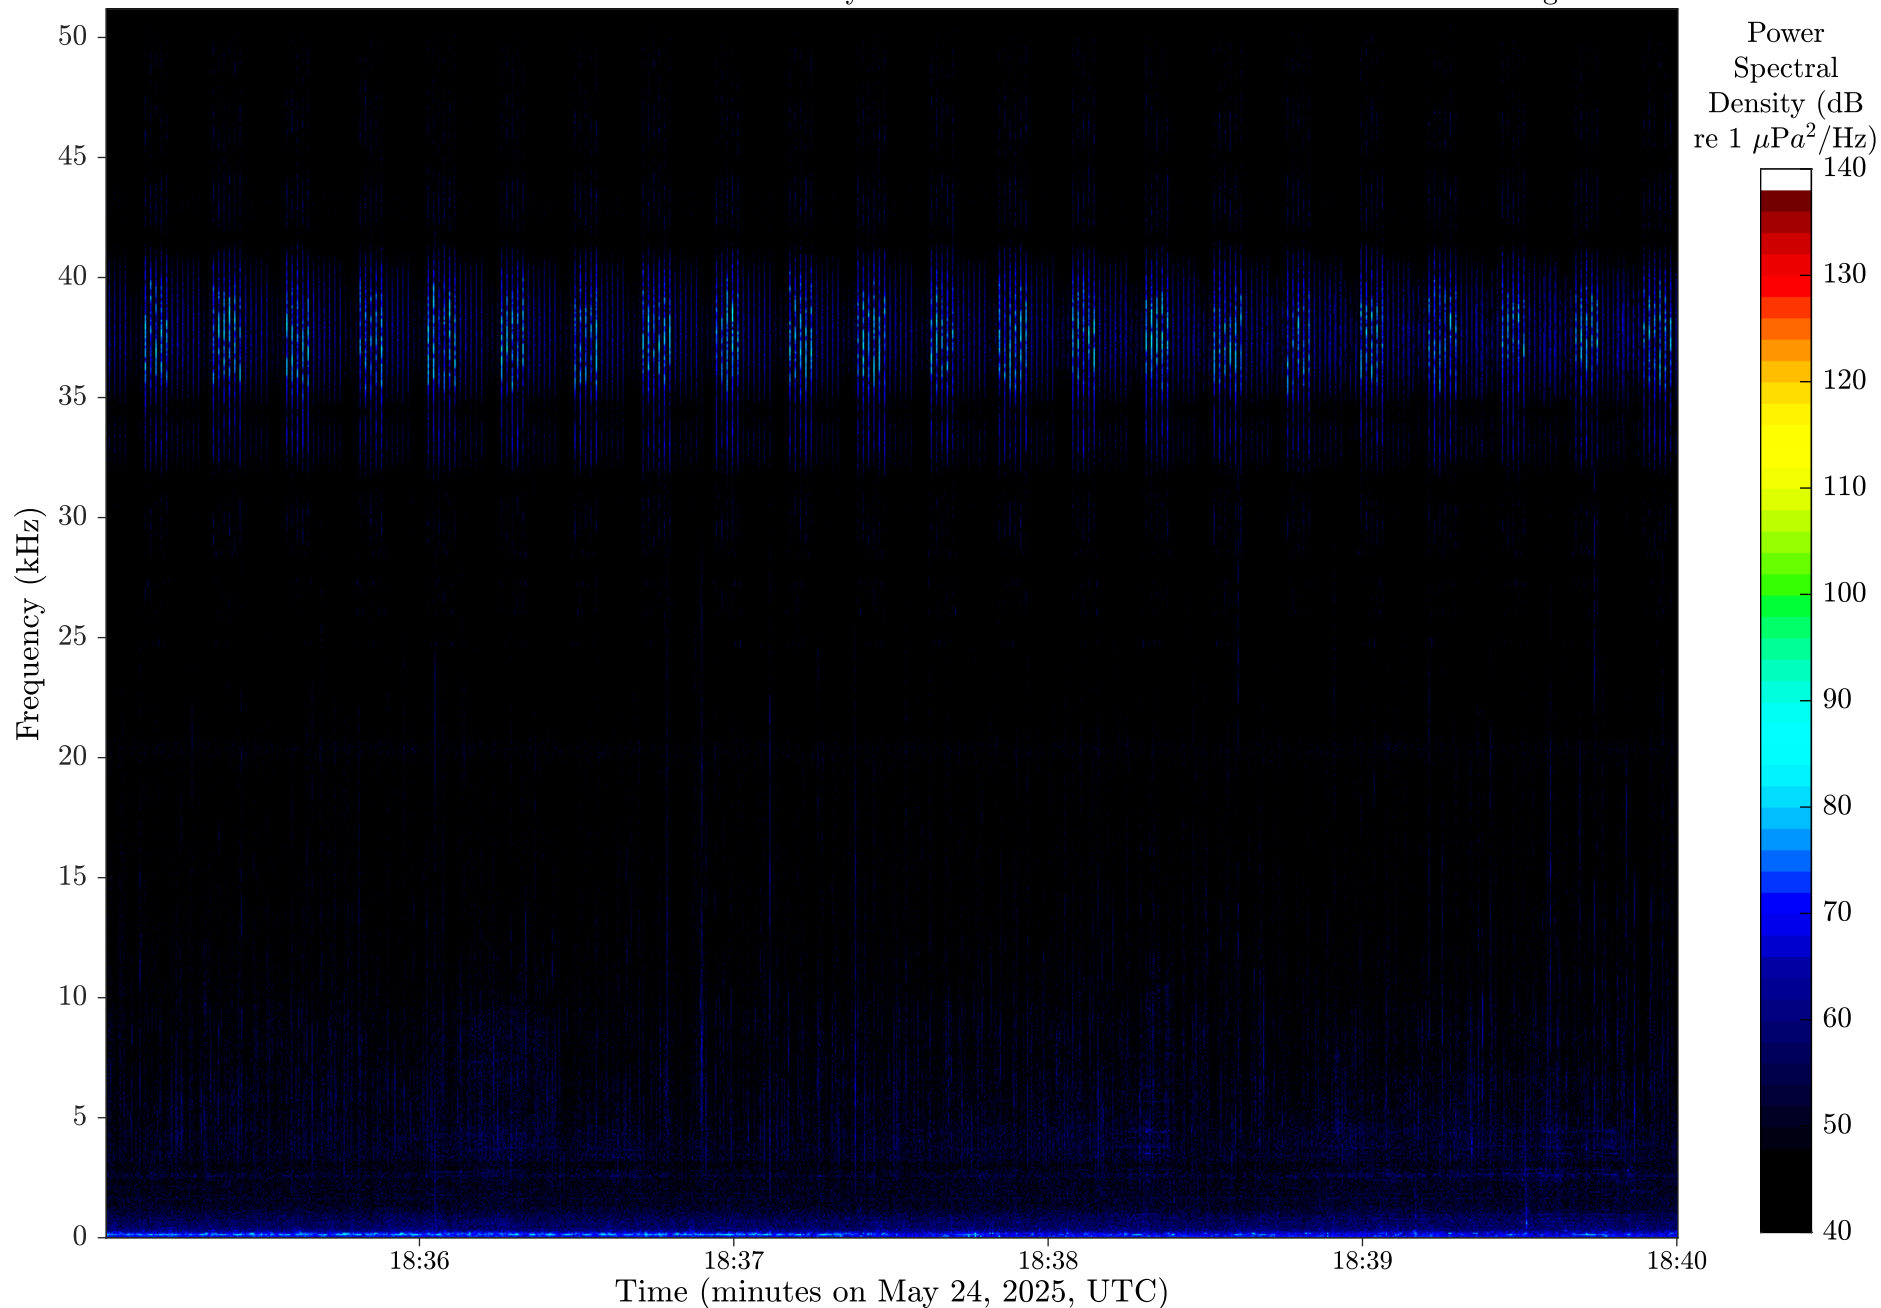


Comments: 31.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:21 UTC

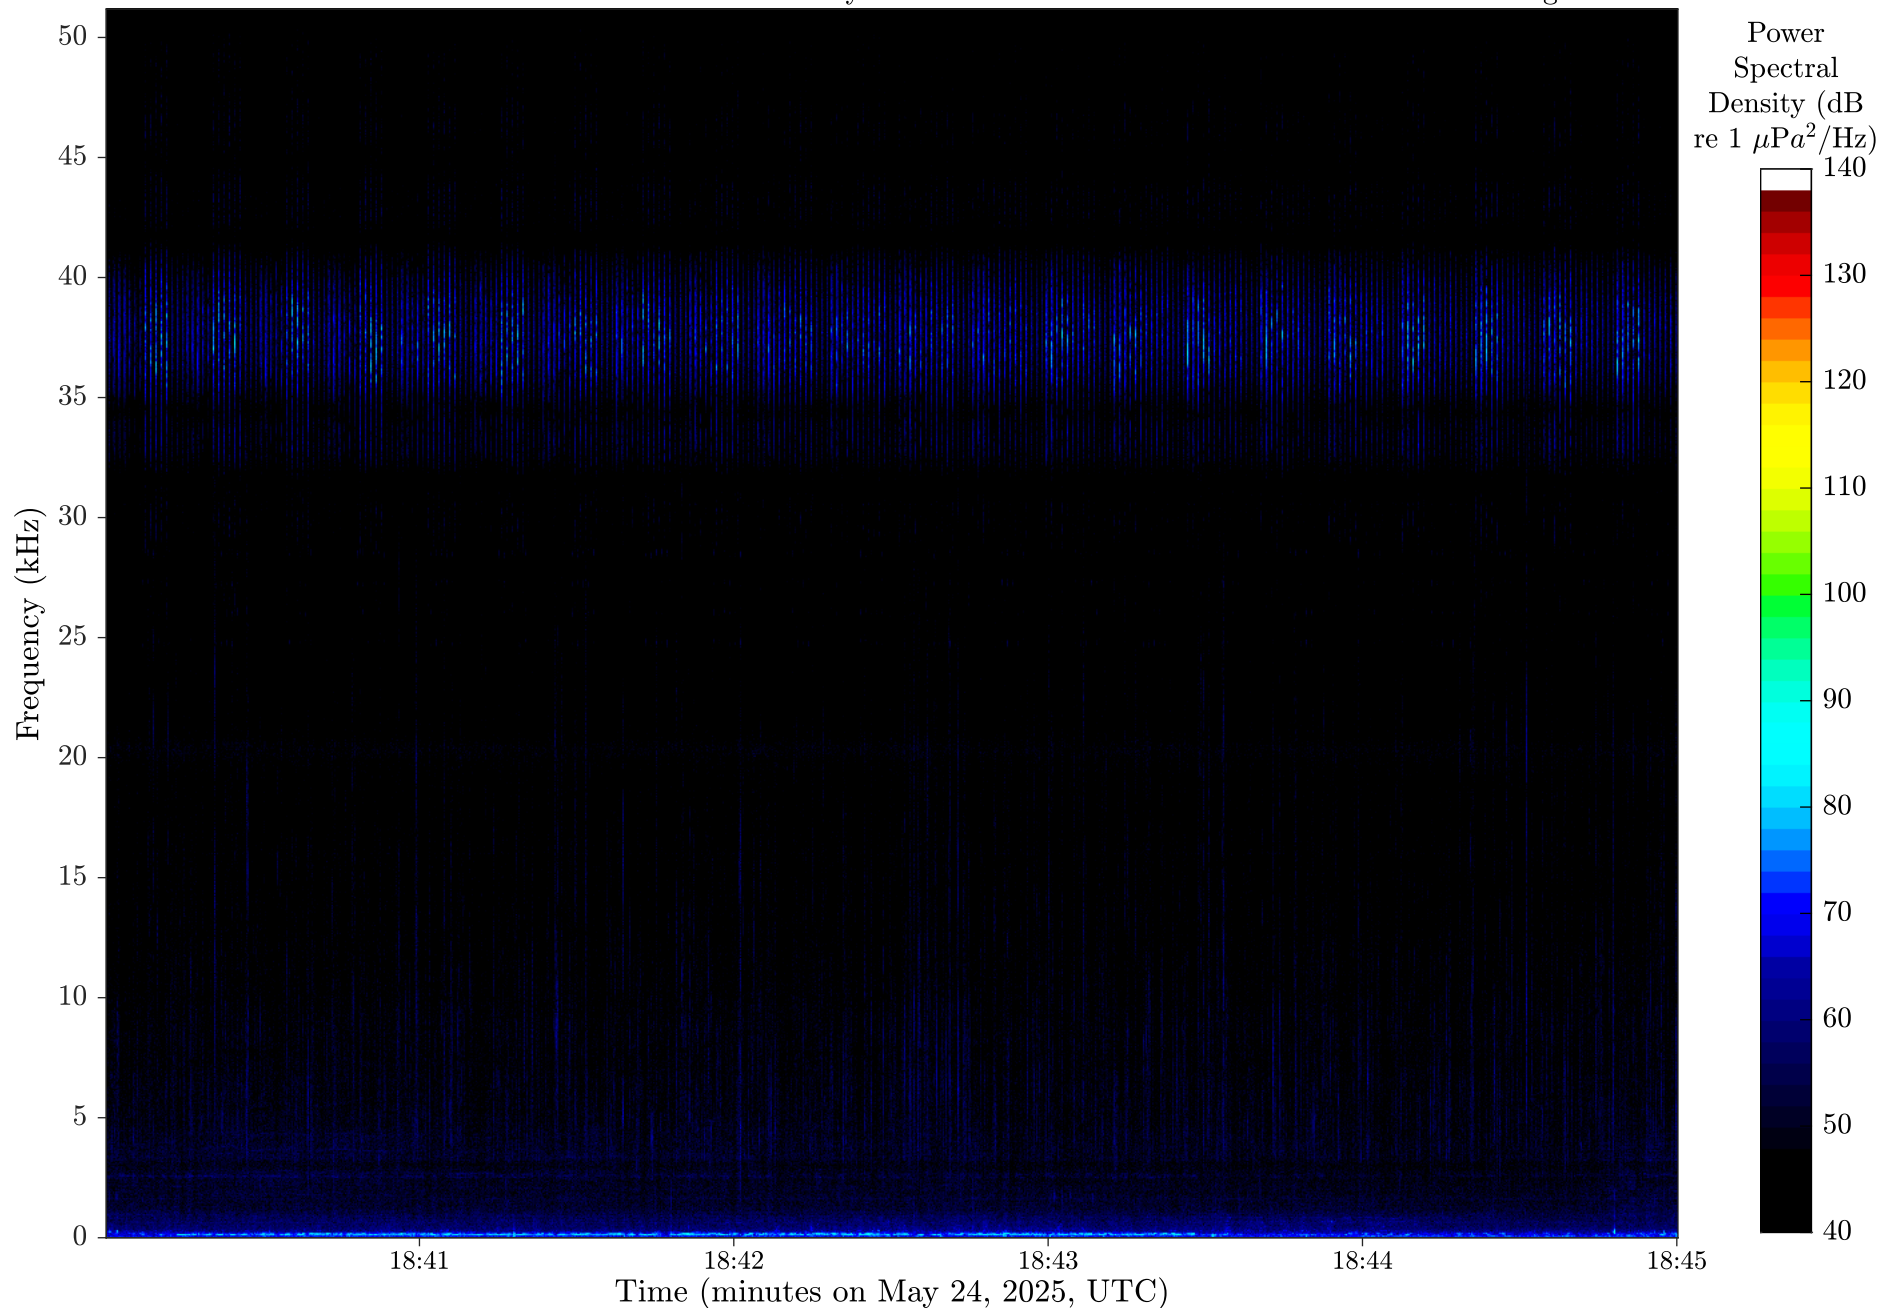


Comments: 30.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:28 UTC

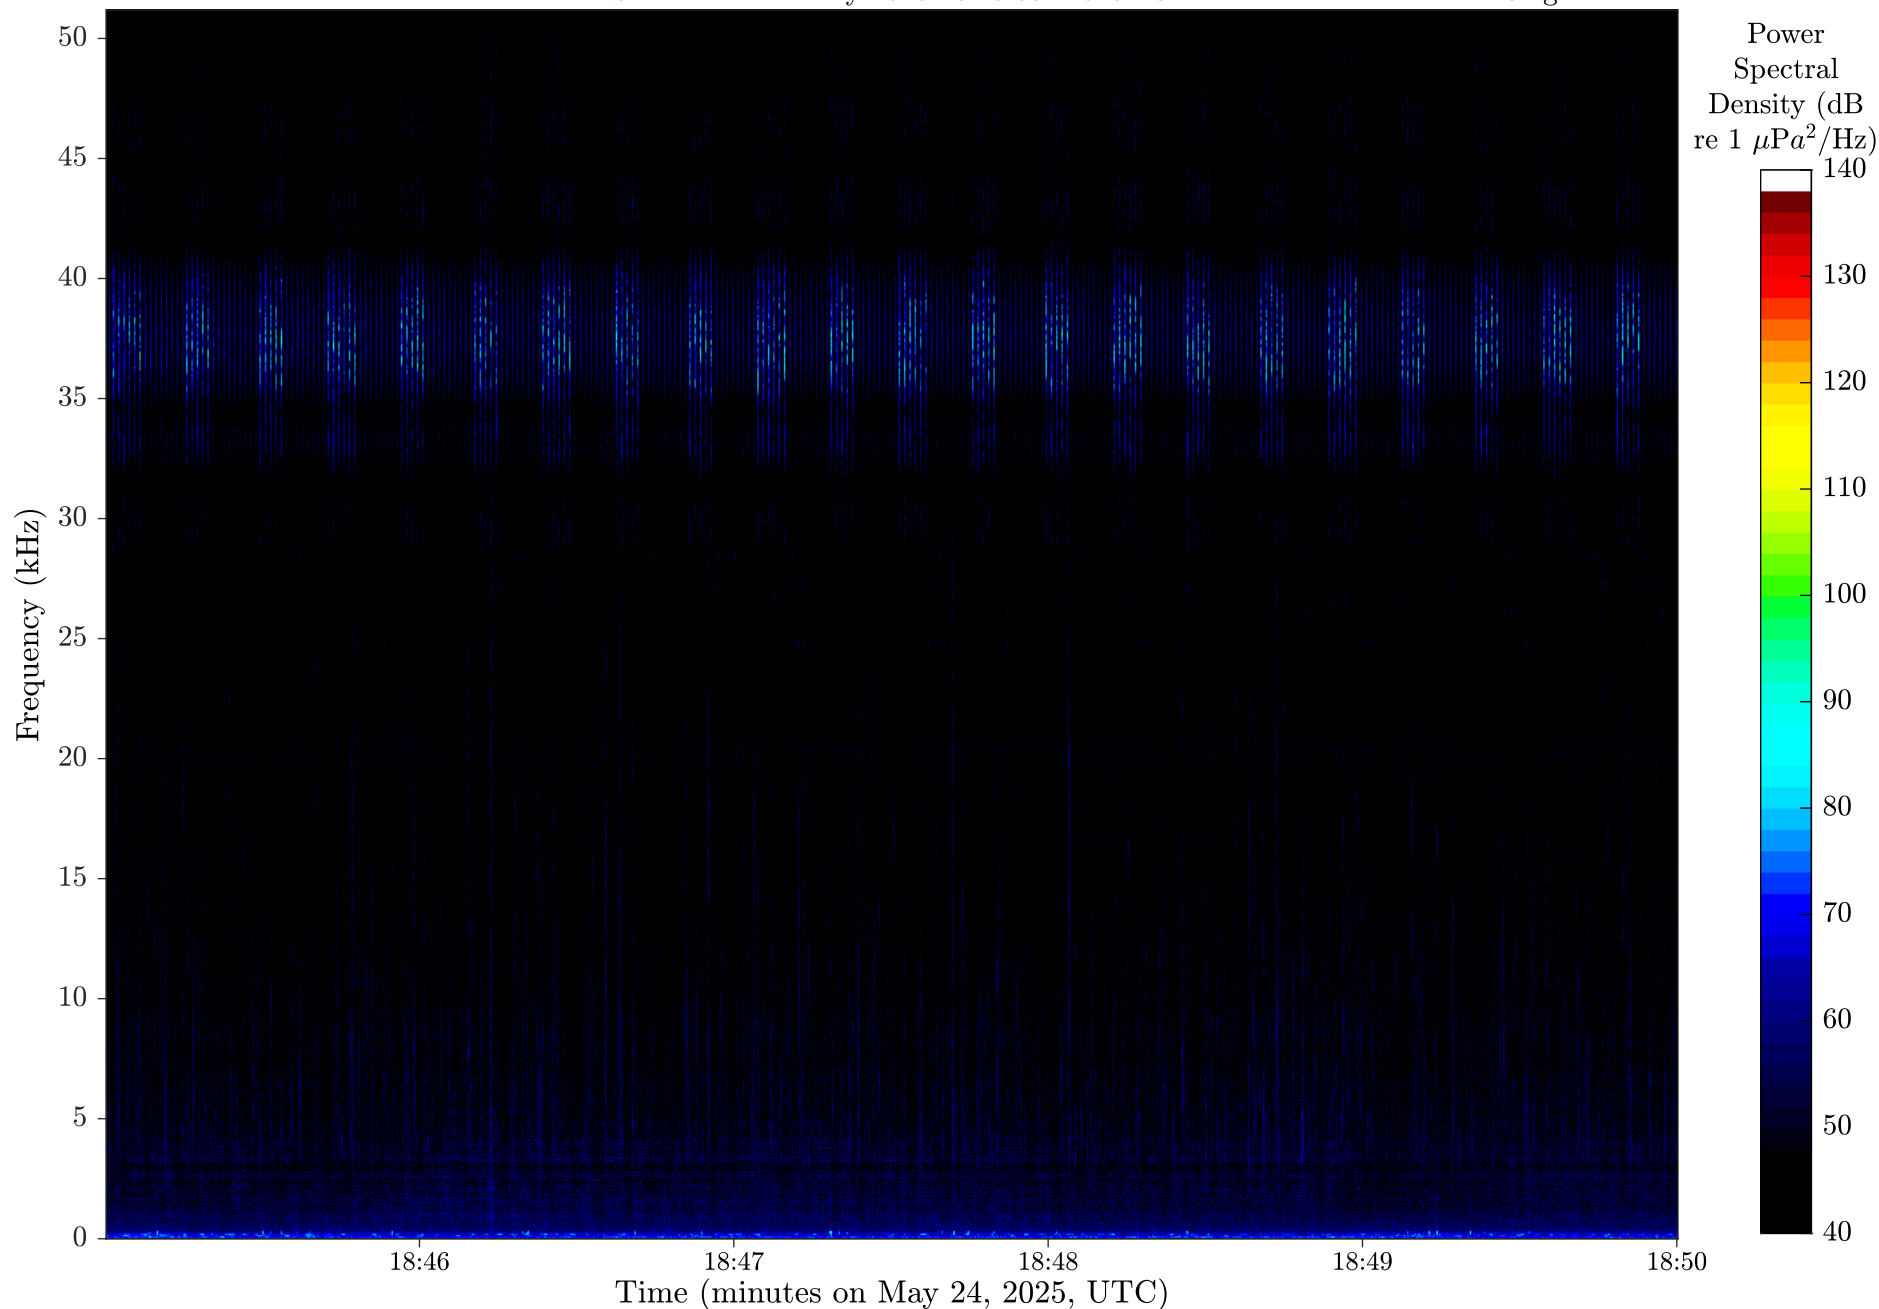


Comments: 31.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:35 UTC

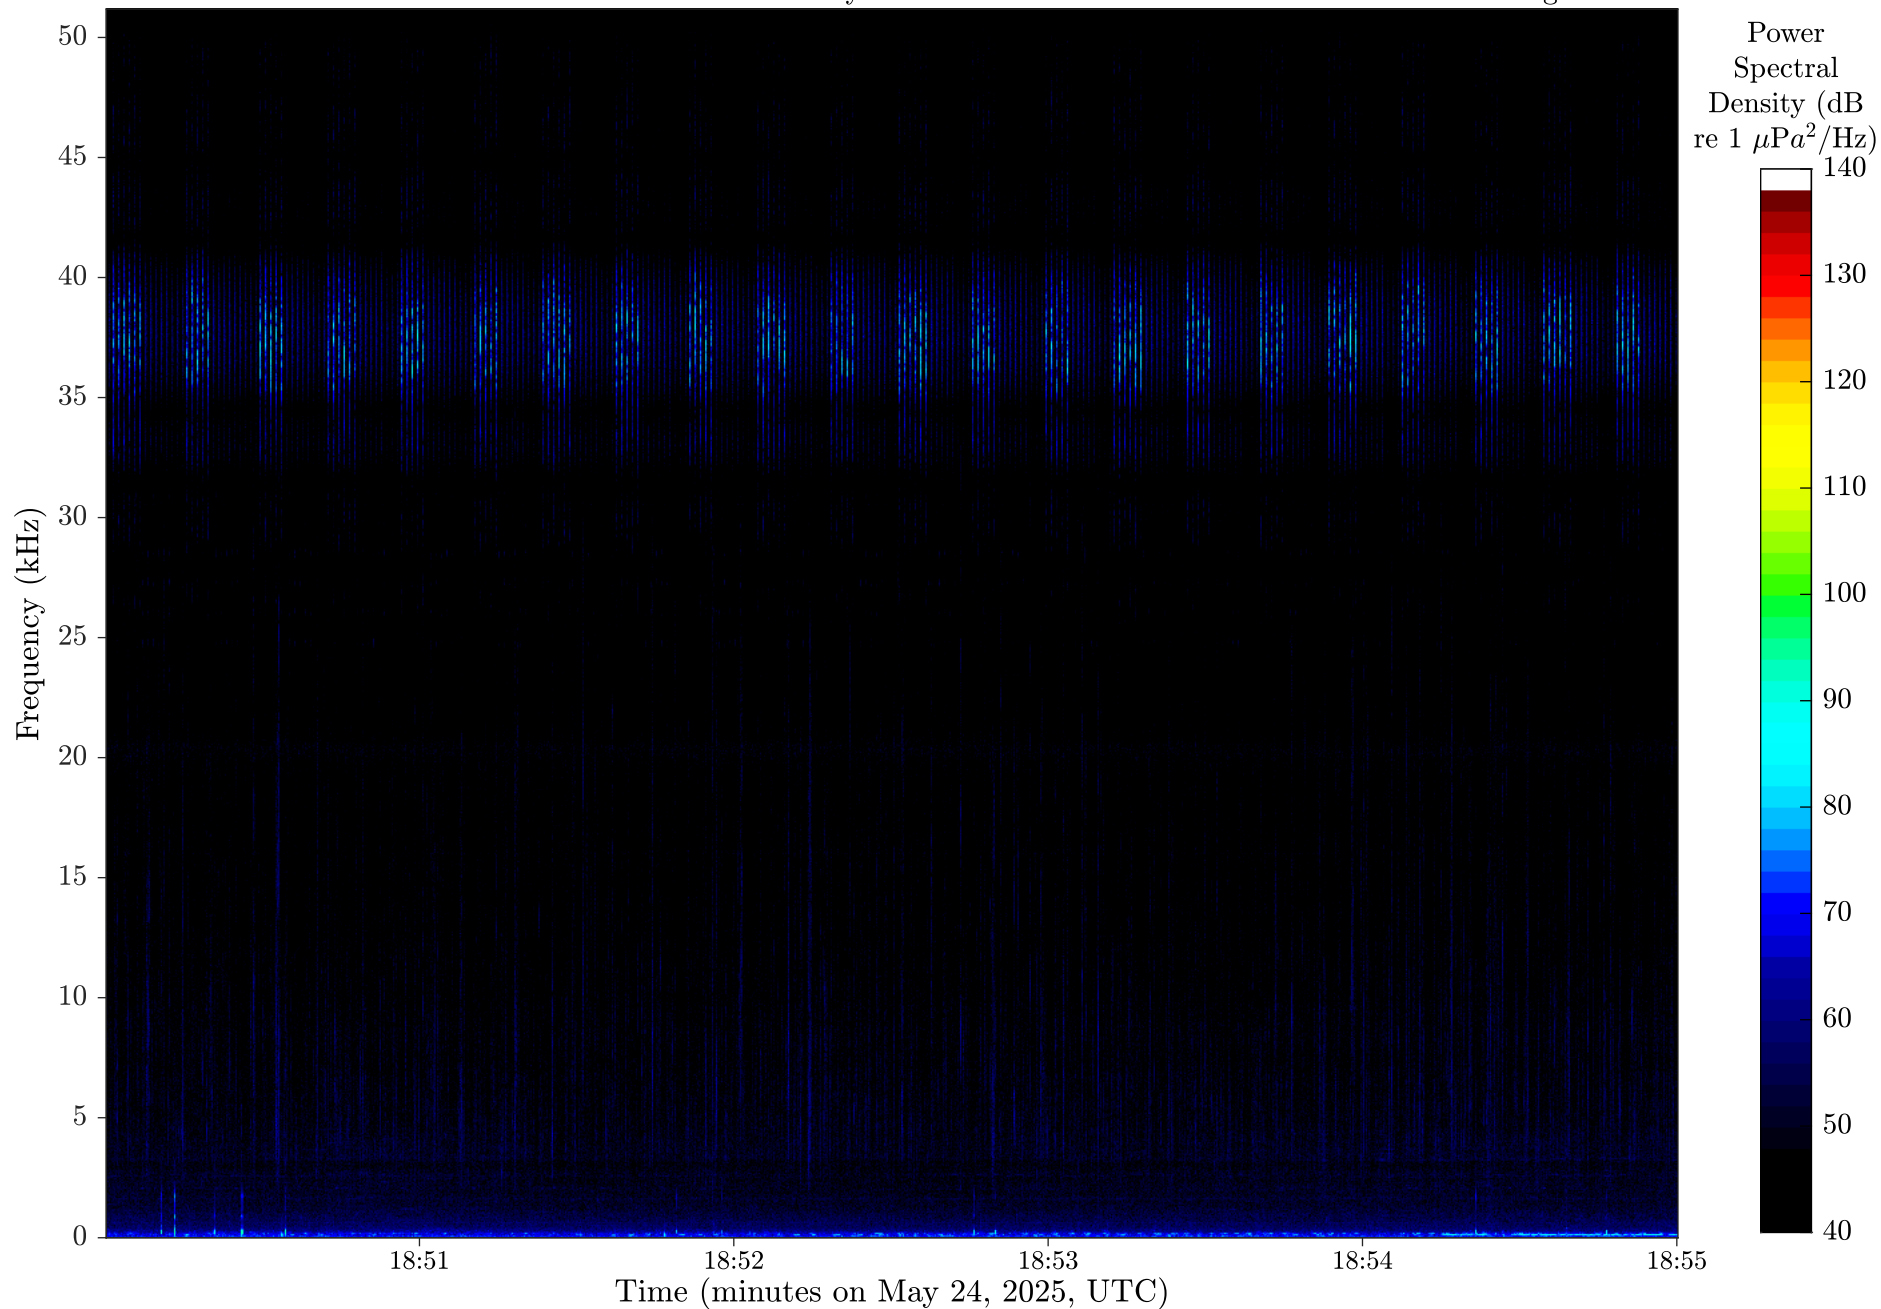


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:42 UTC

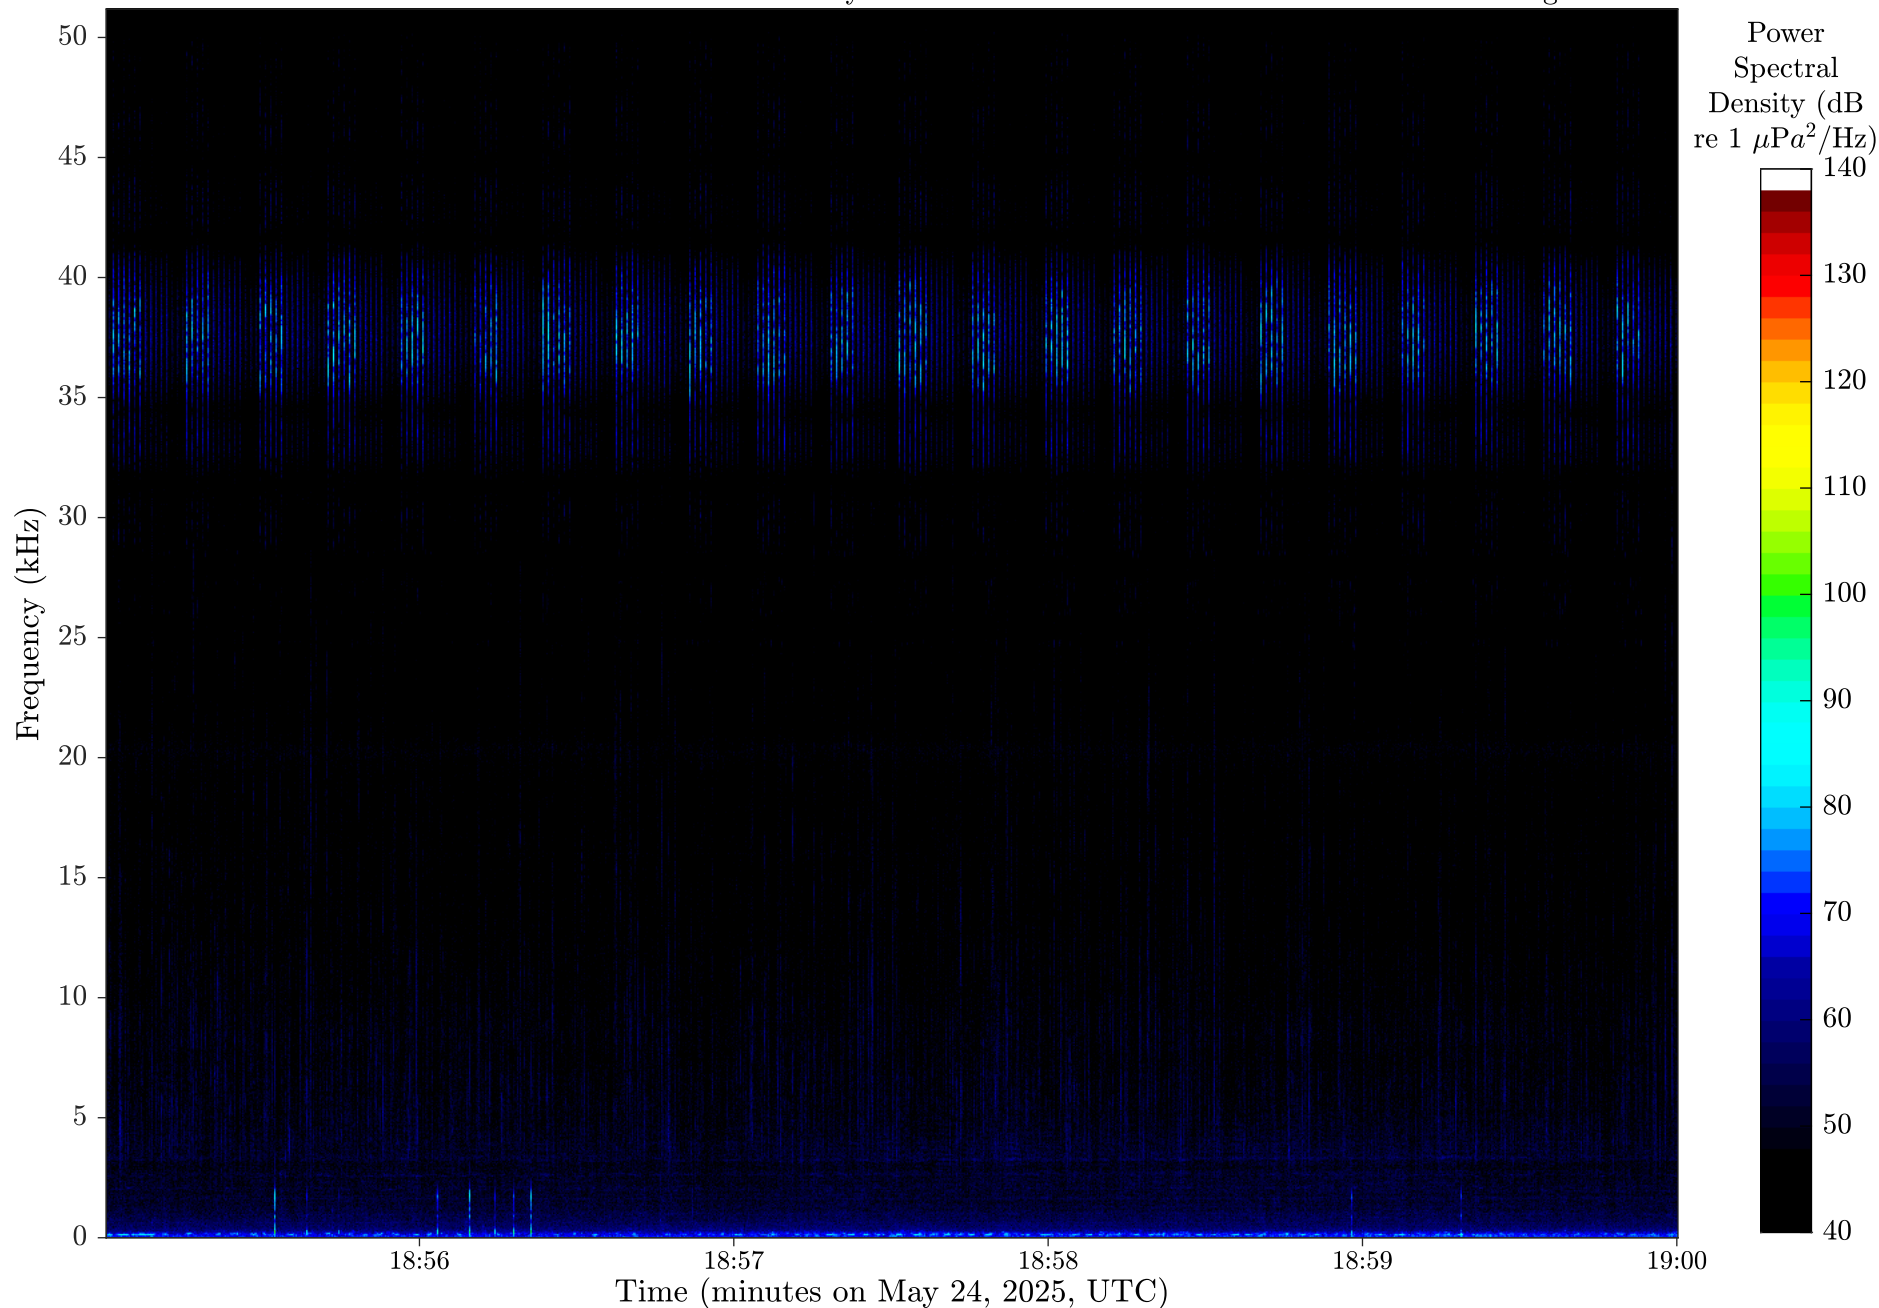


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:50 UTC

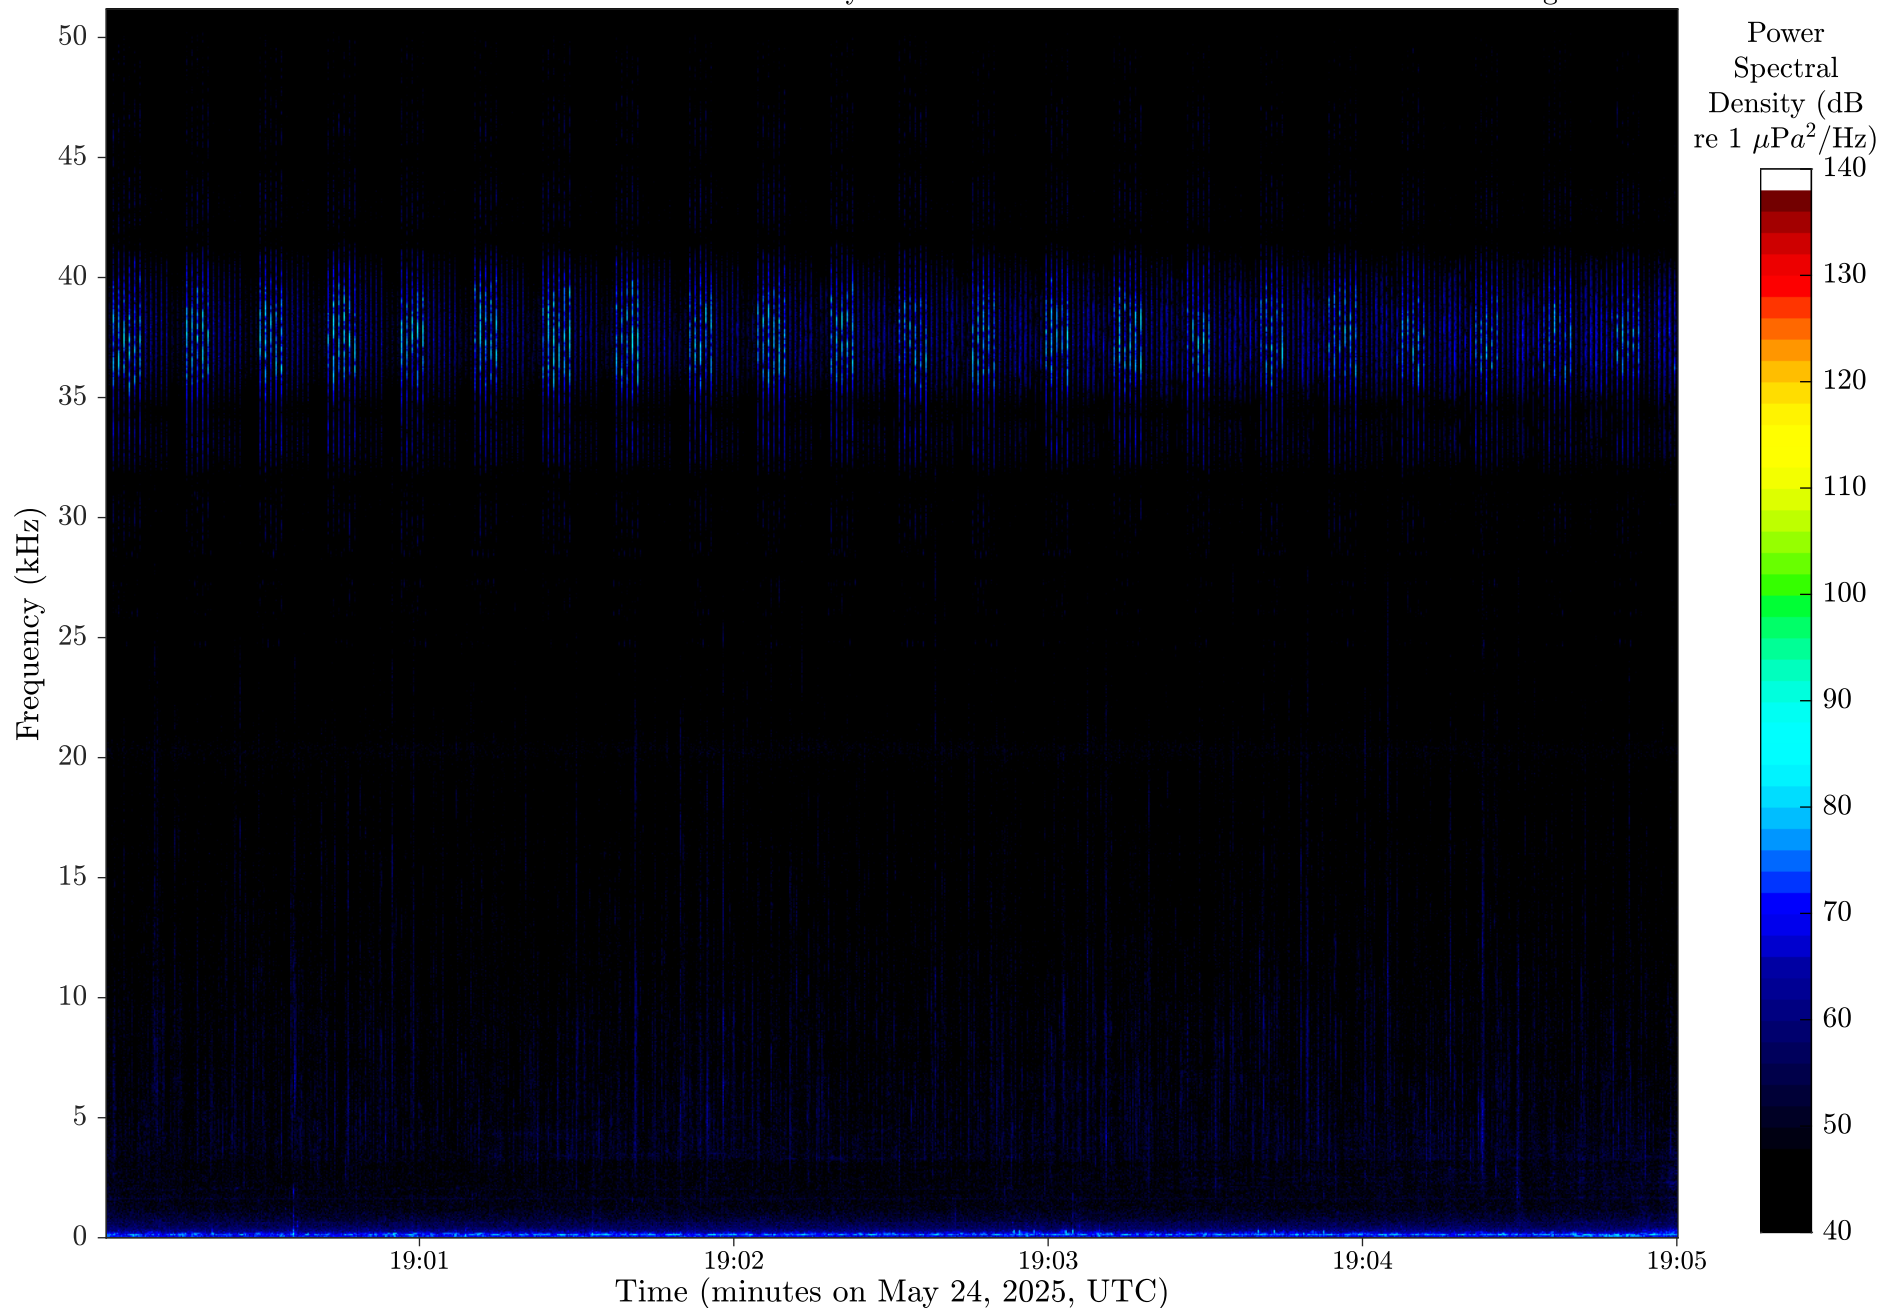


Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:39:57 UTC

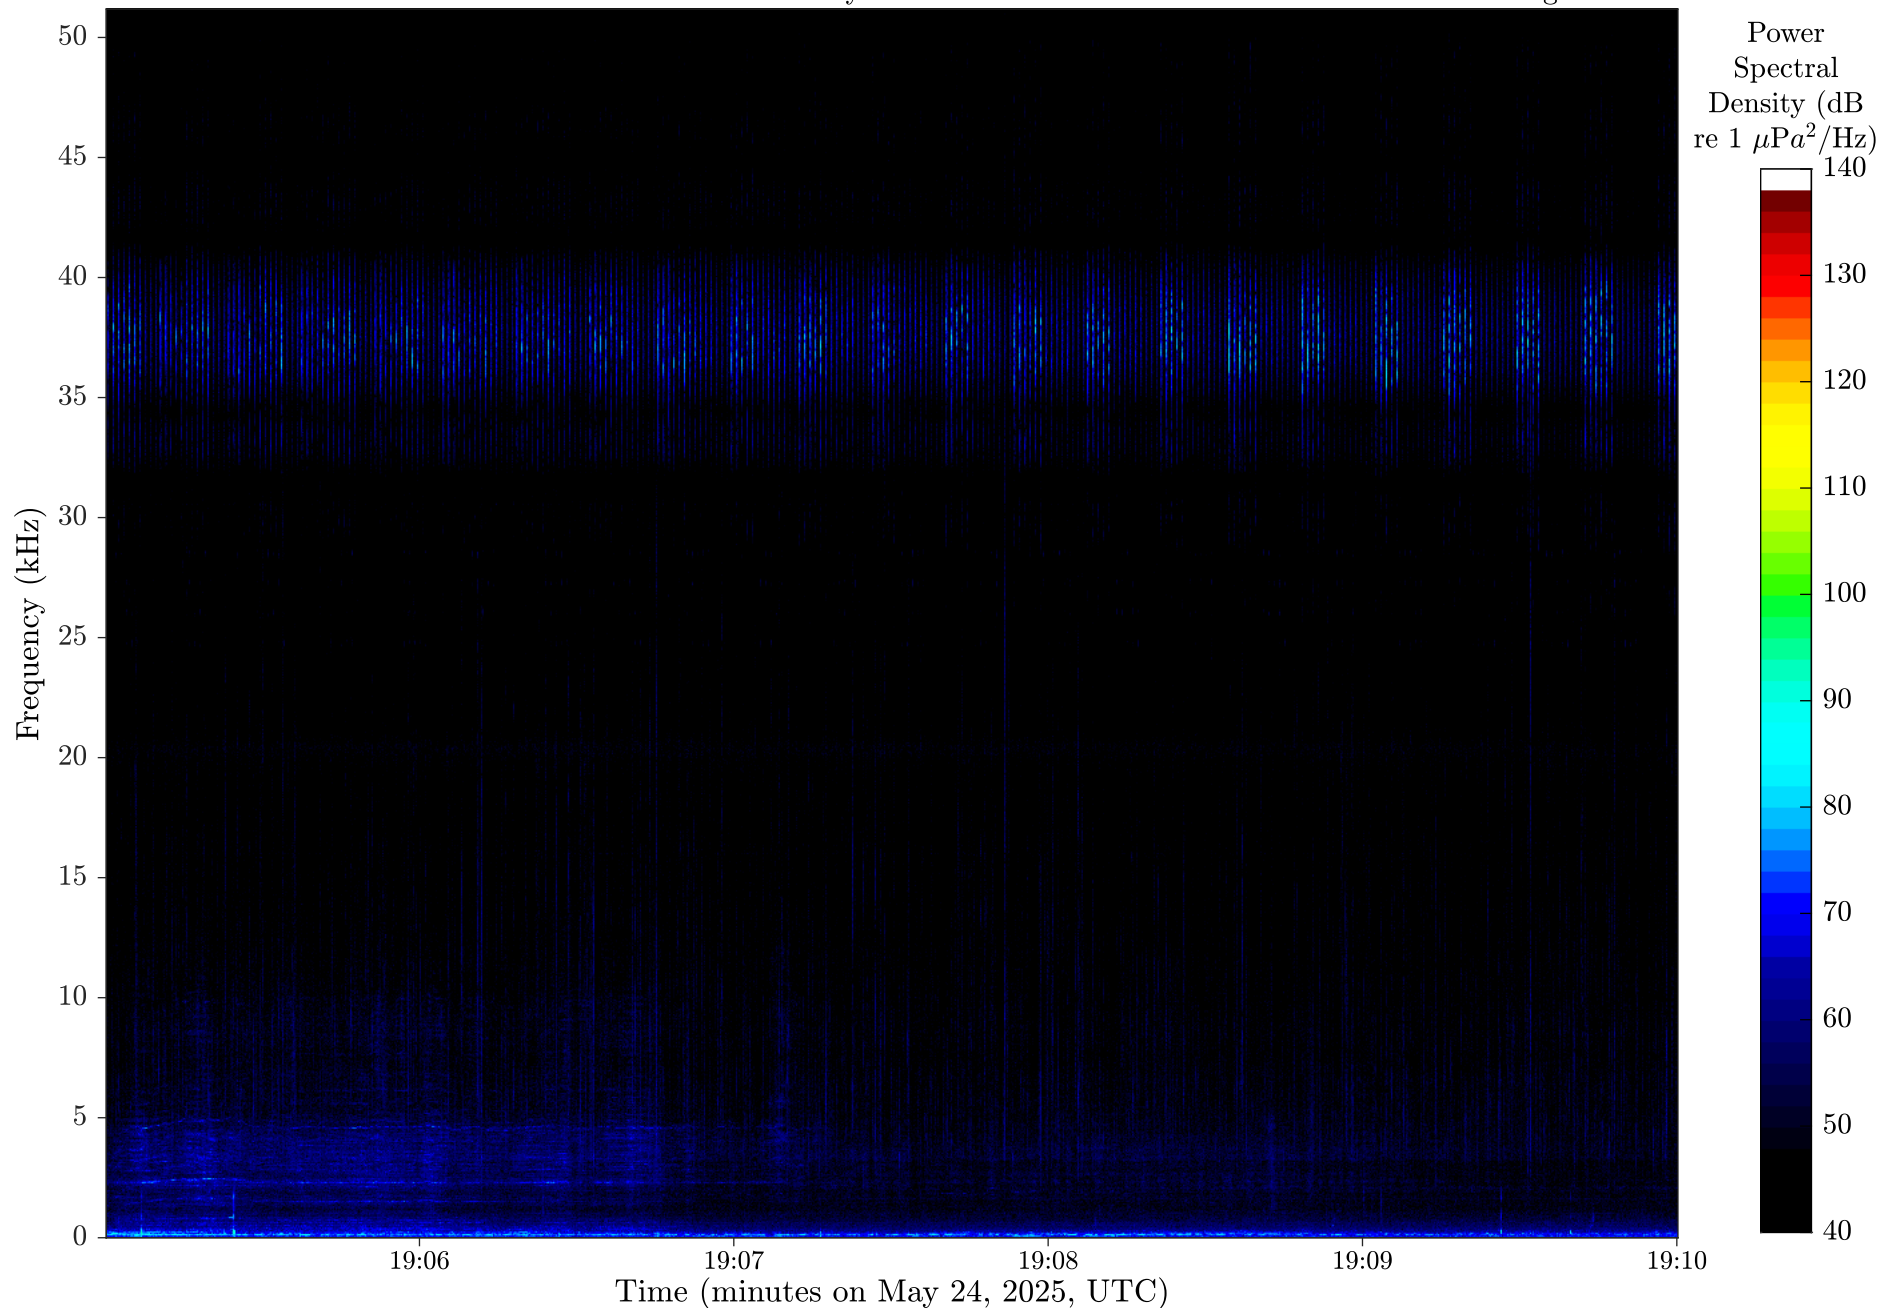

Comments: 32.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:40:04 UTC

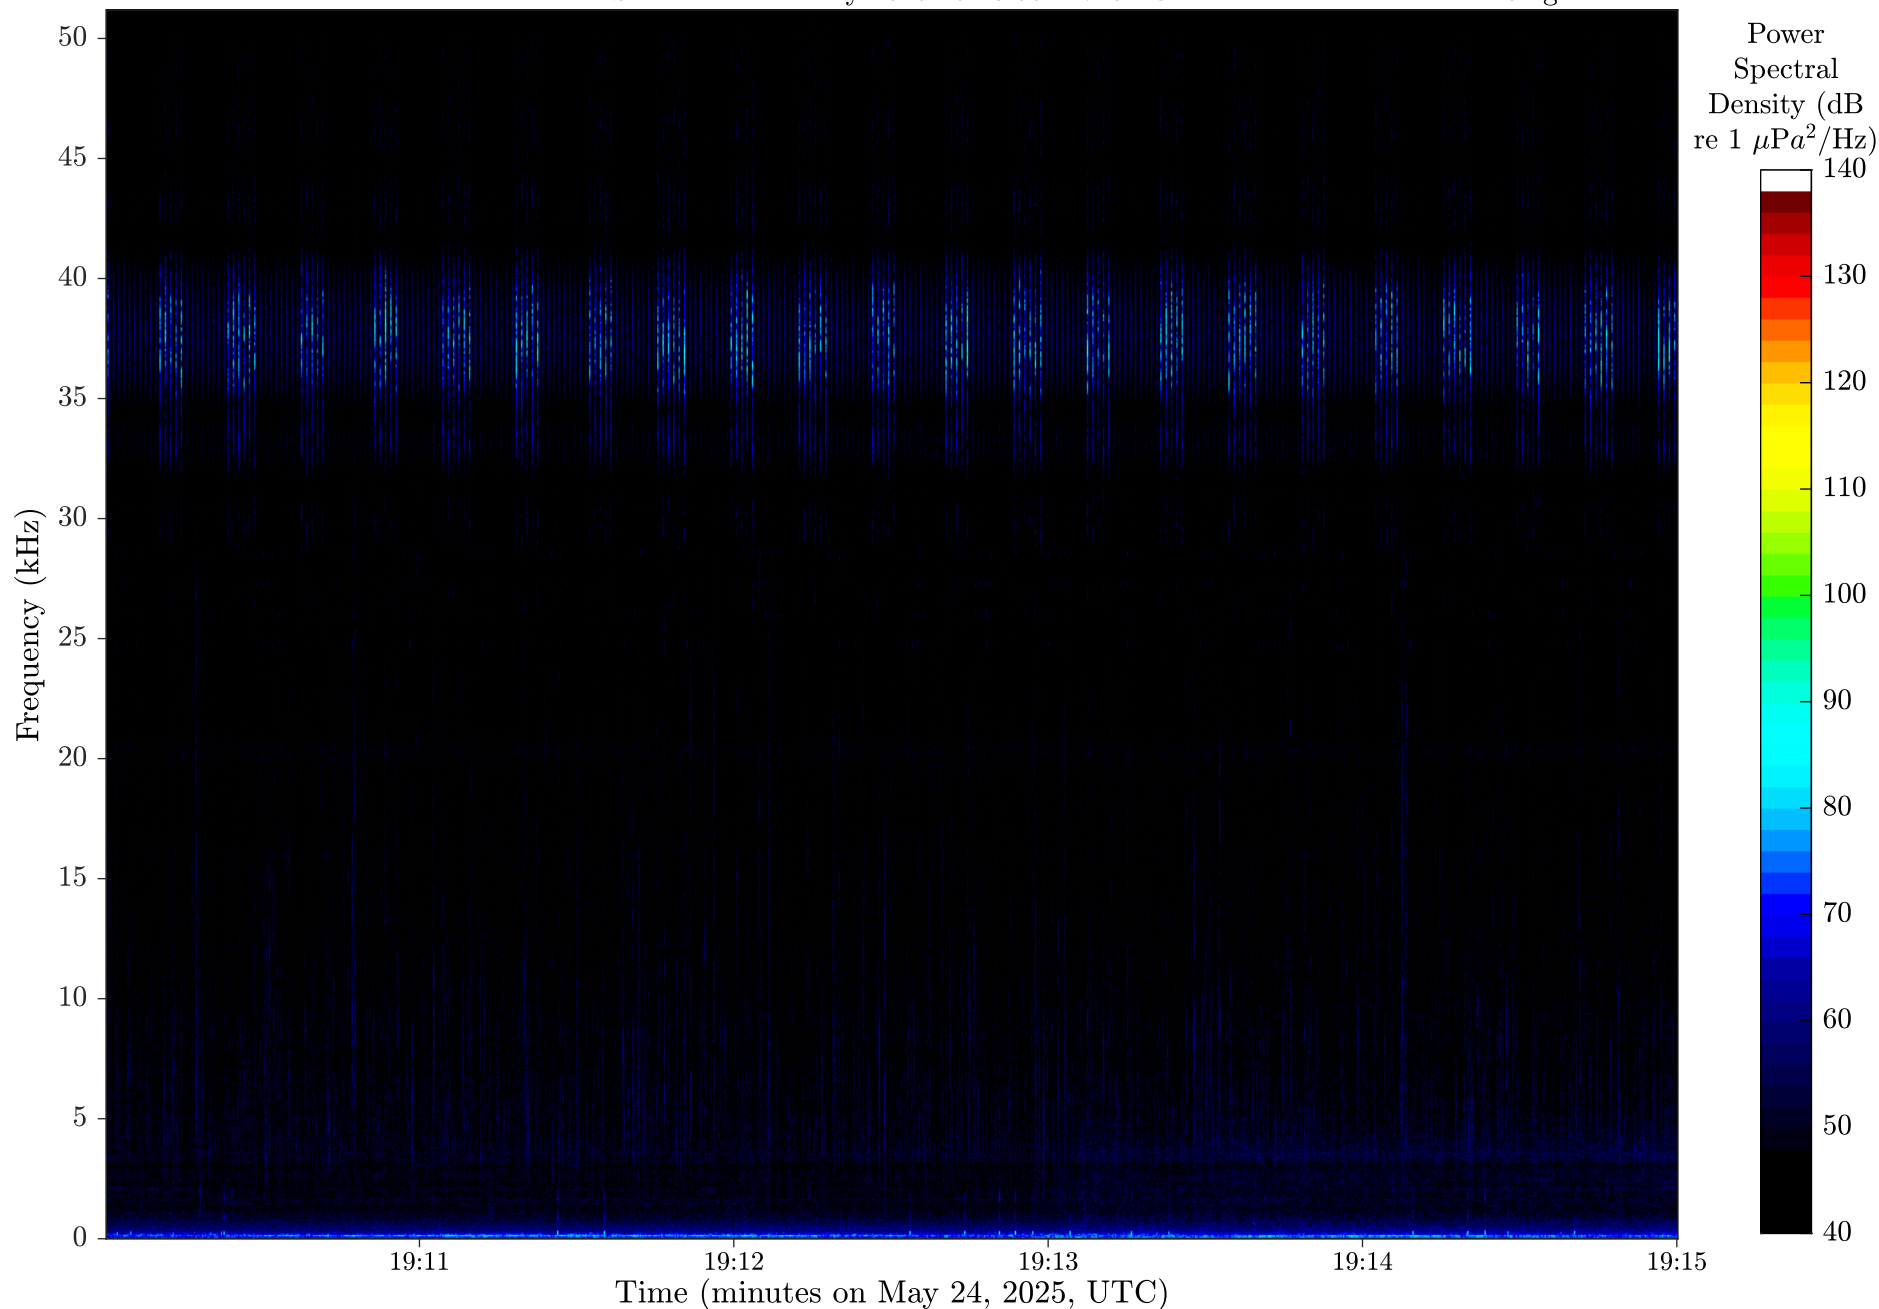

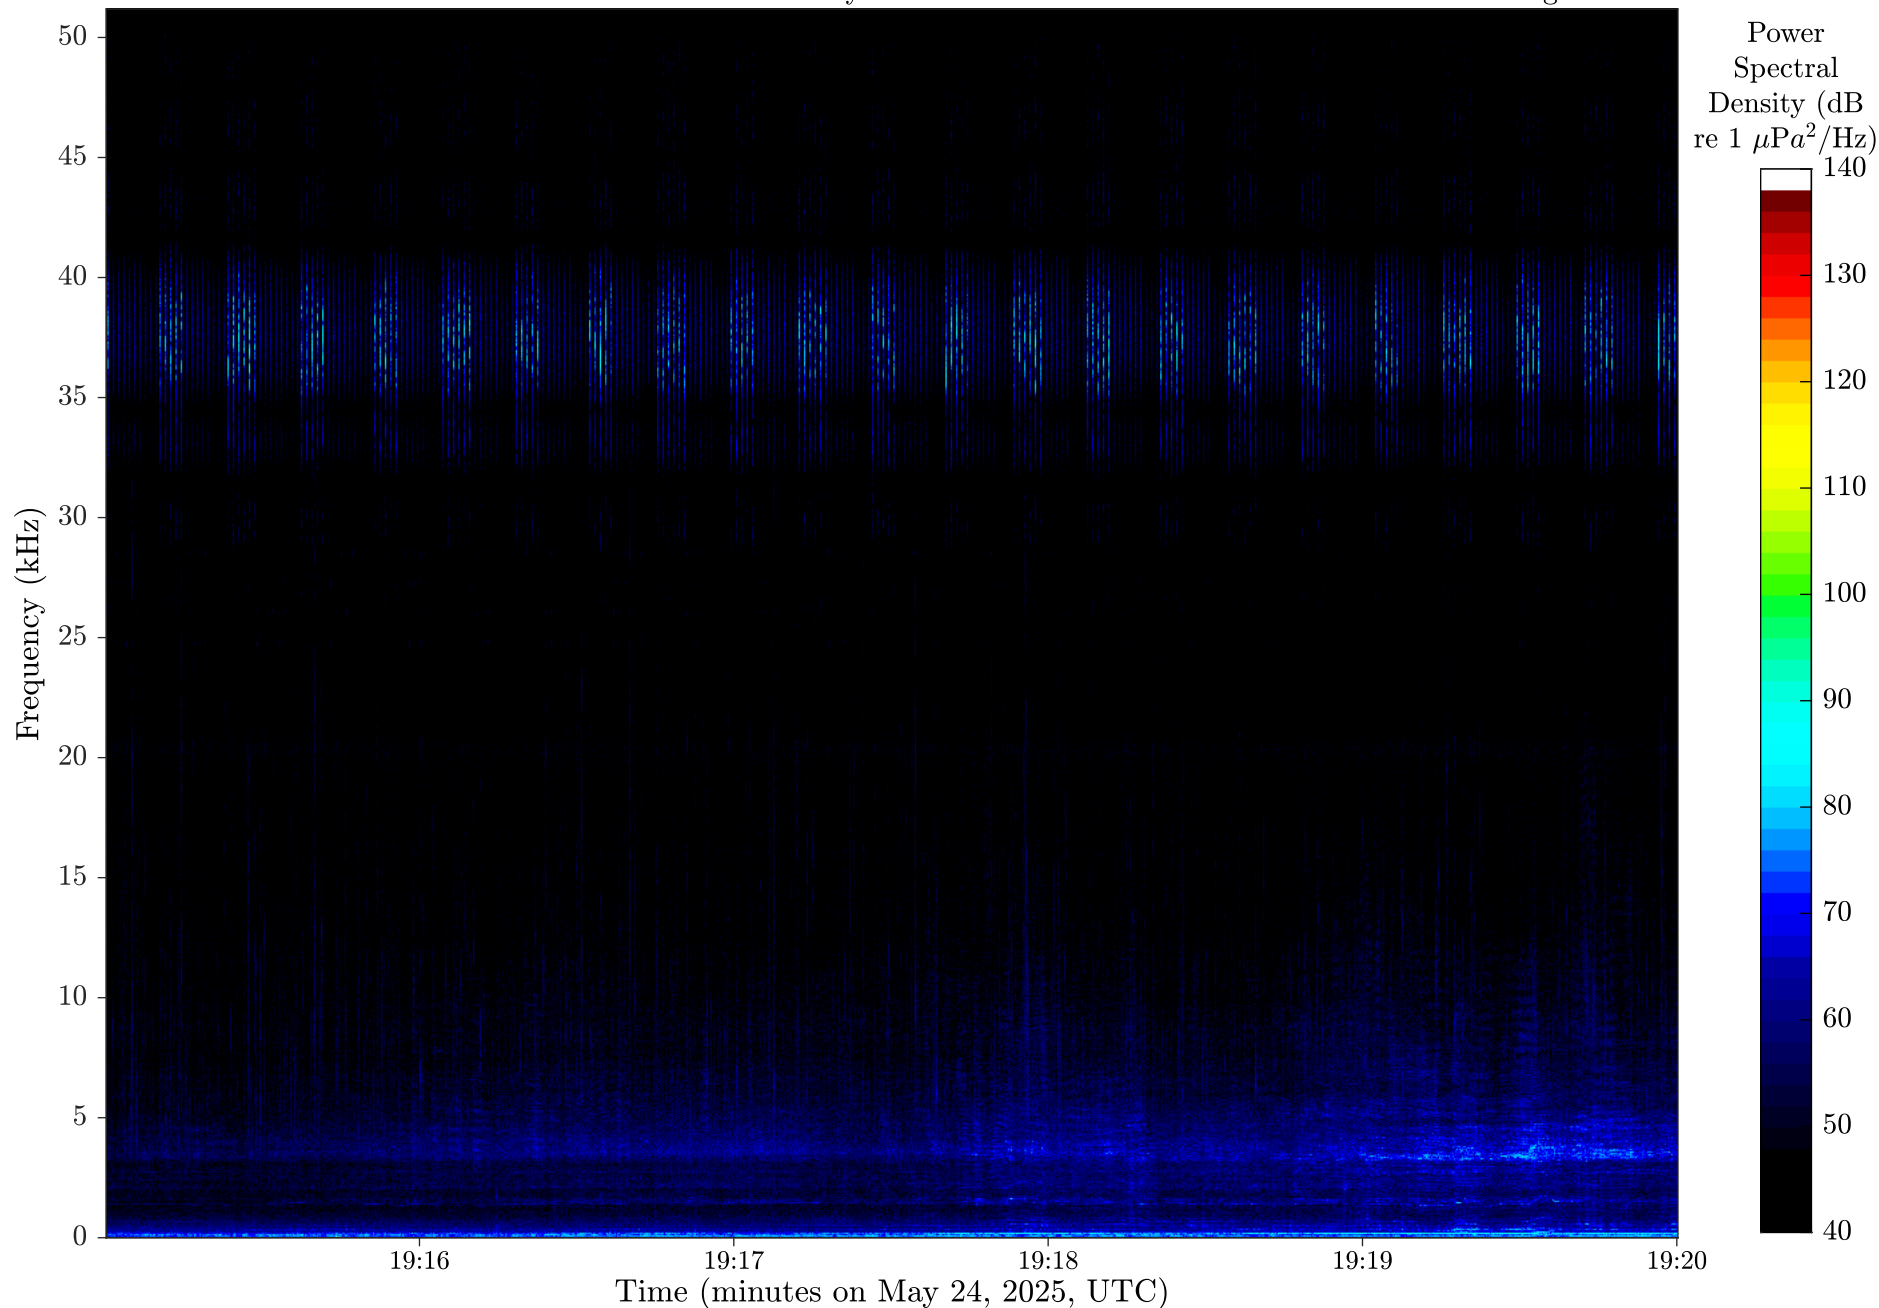


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:17 UTC

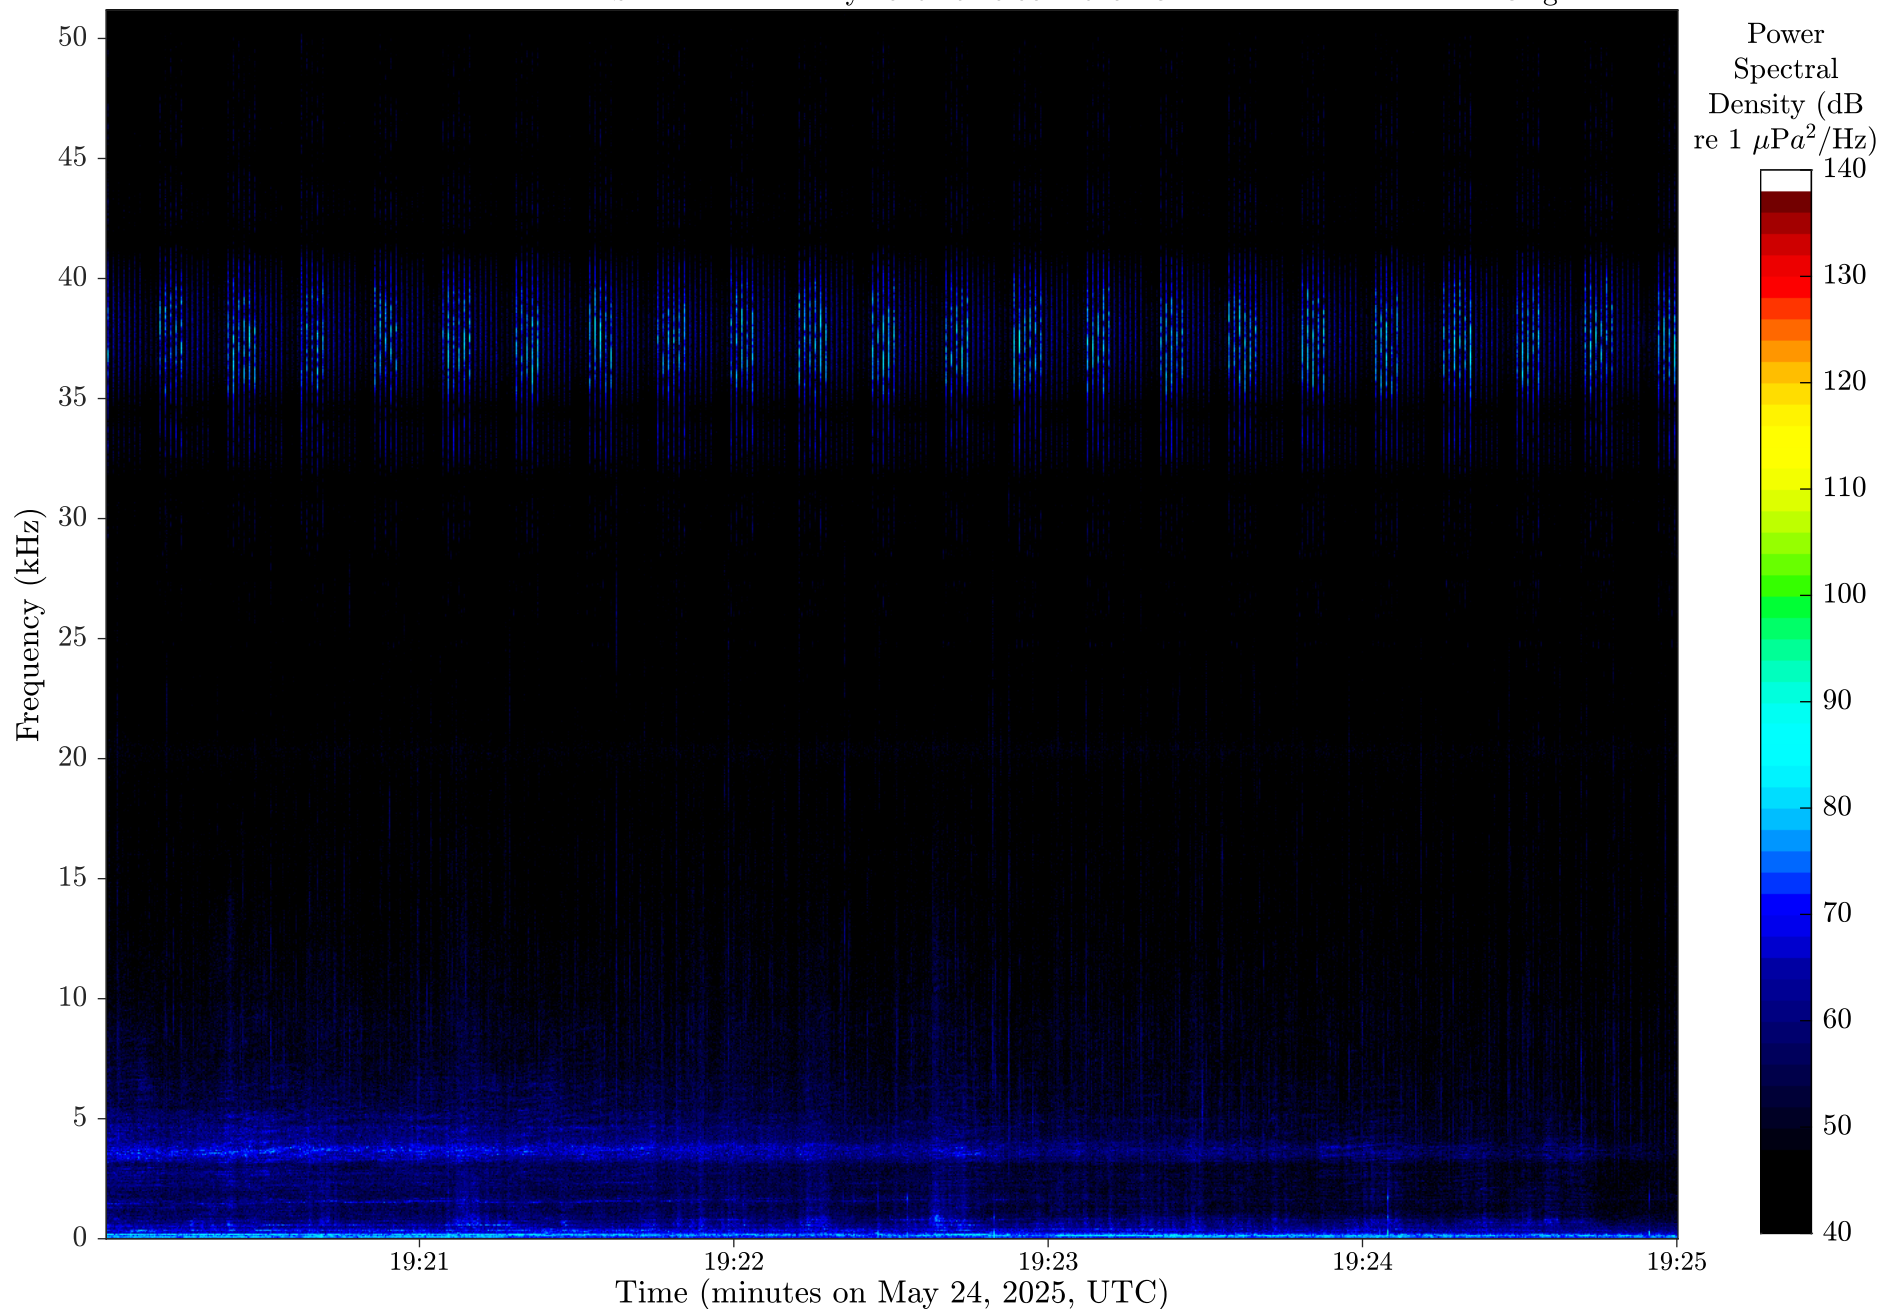


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:24 UTC

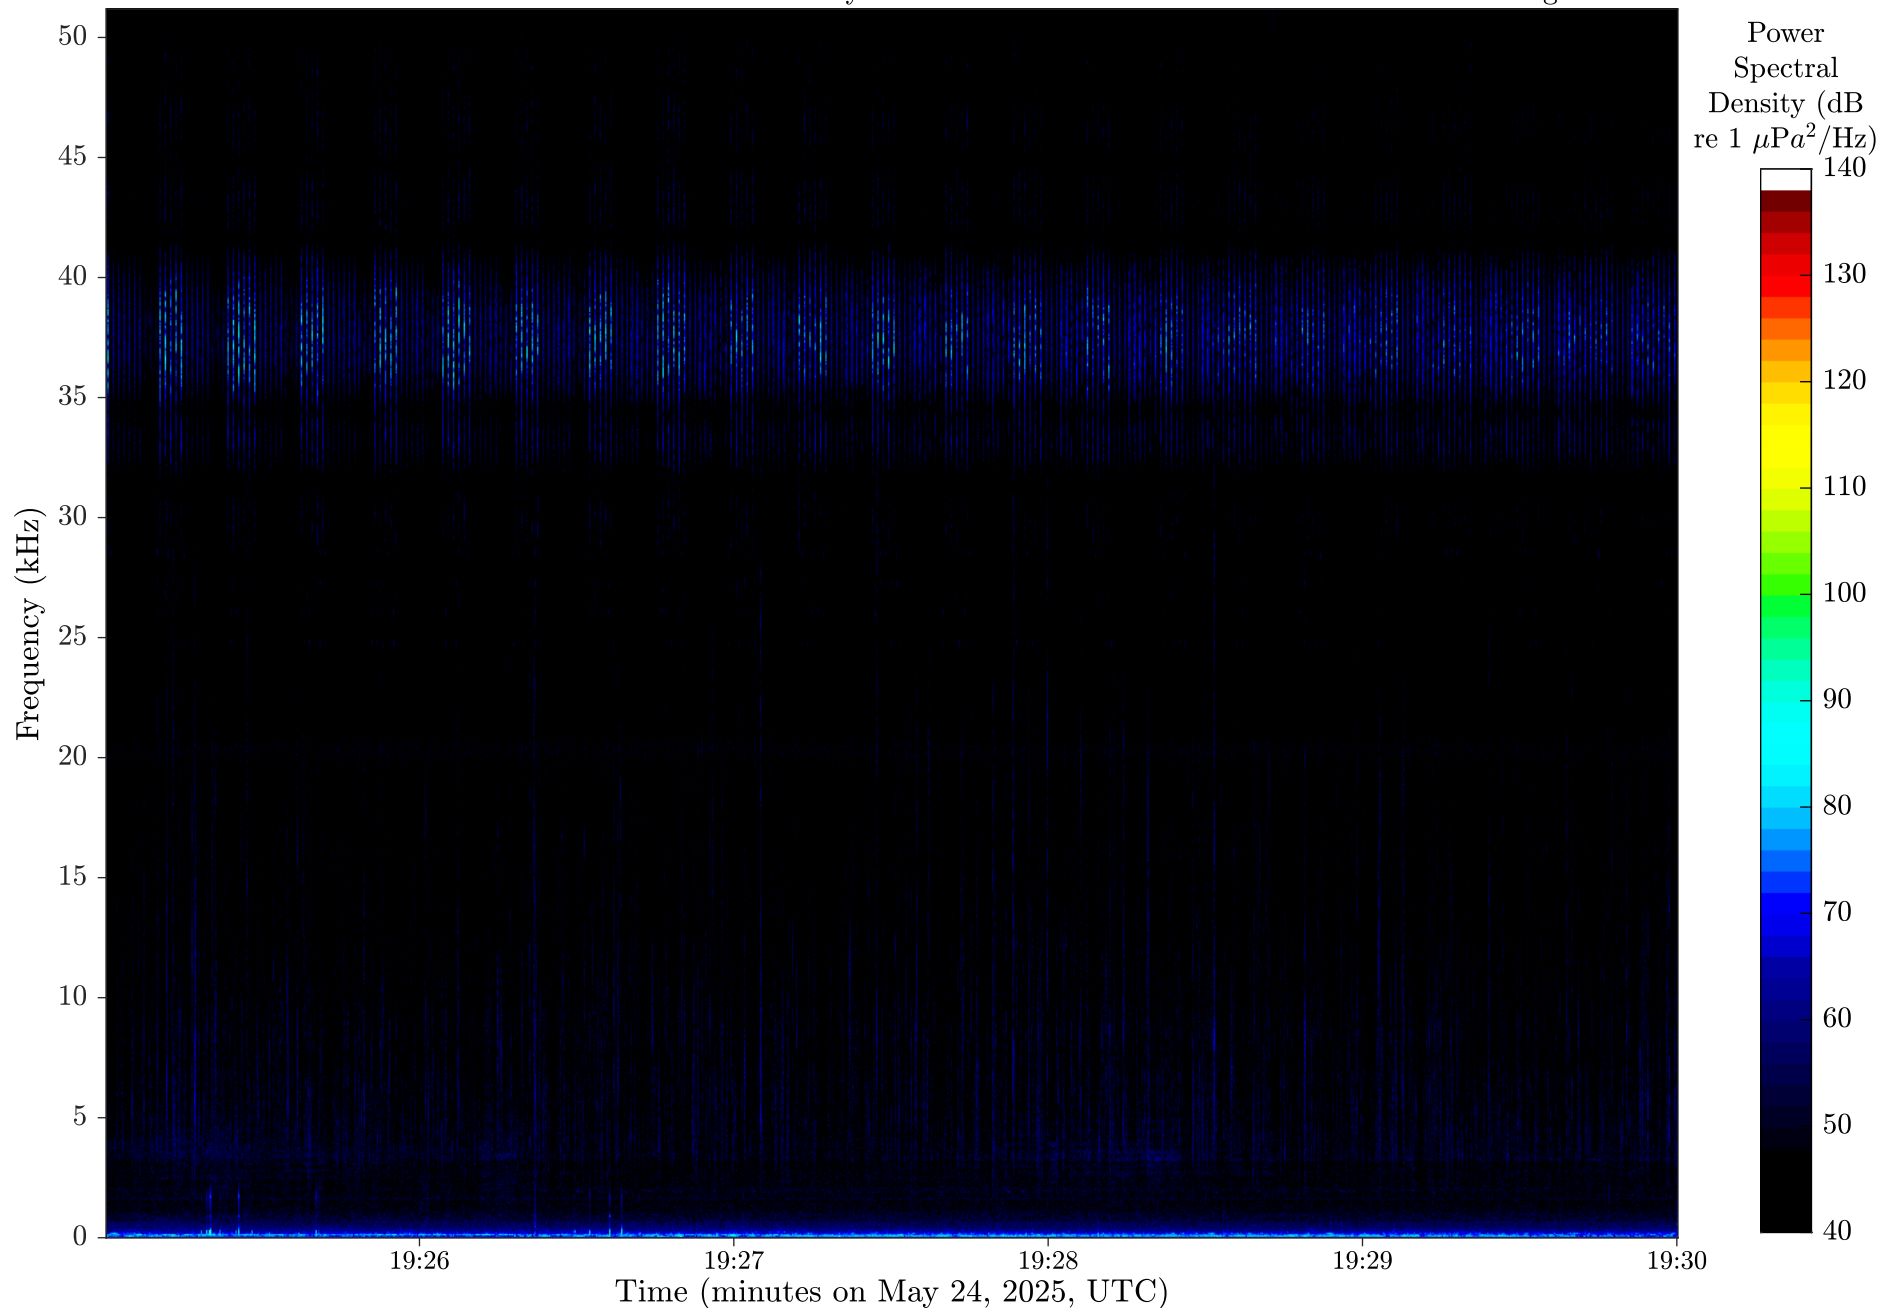


Comments: 33.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:31 UTC

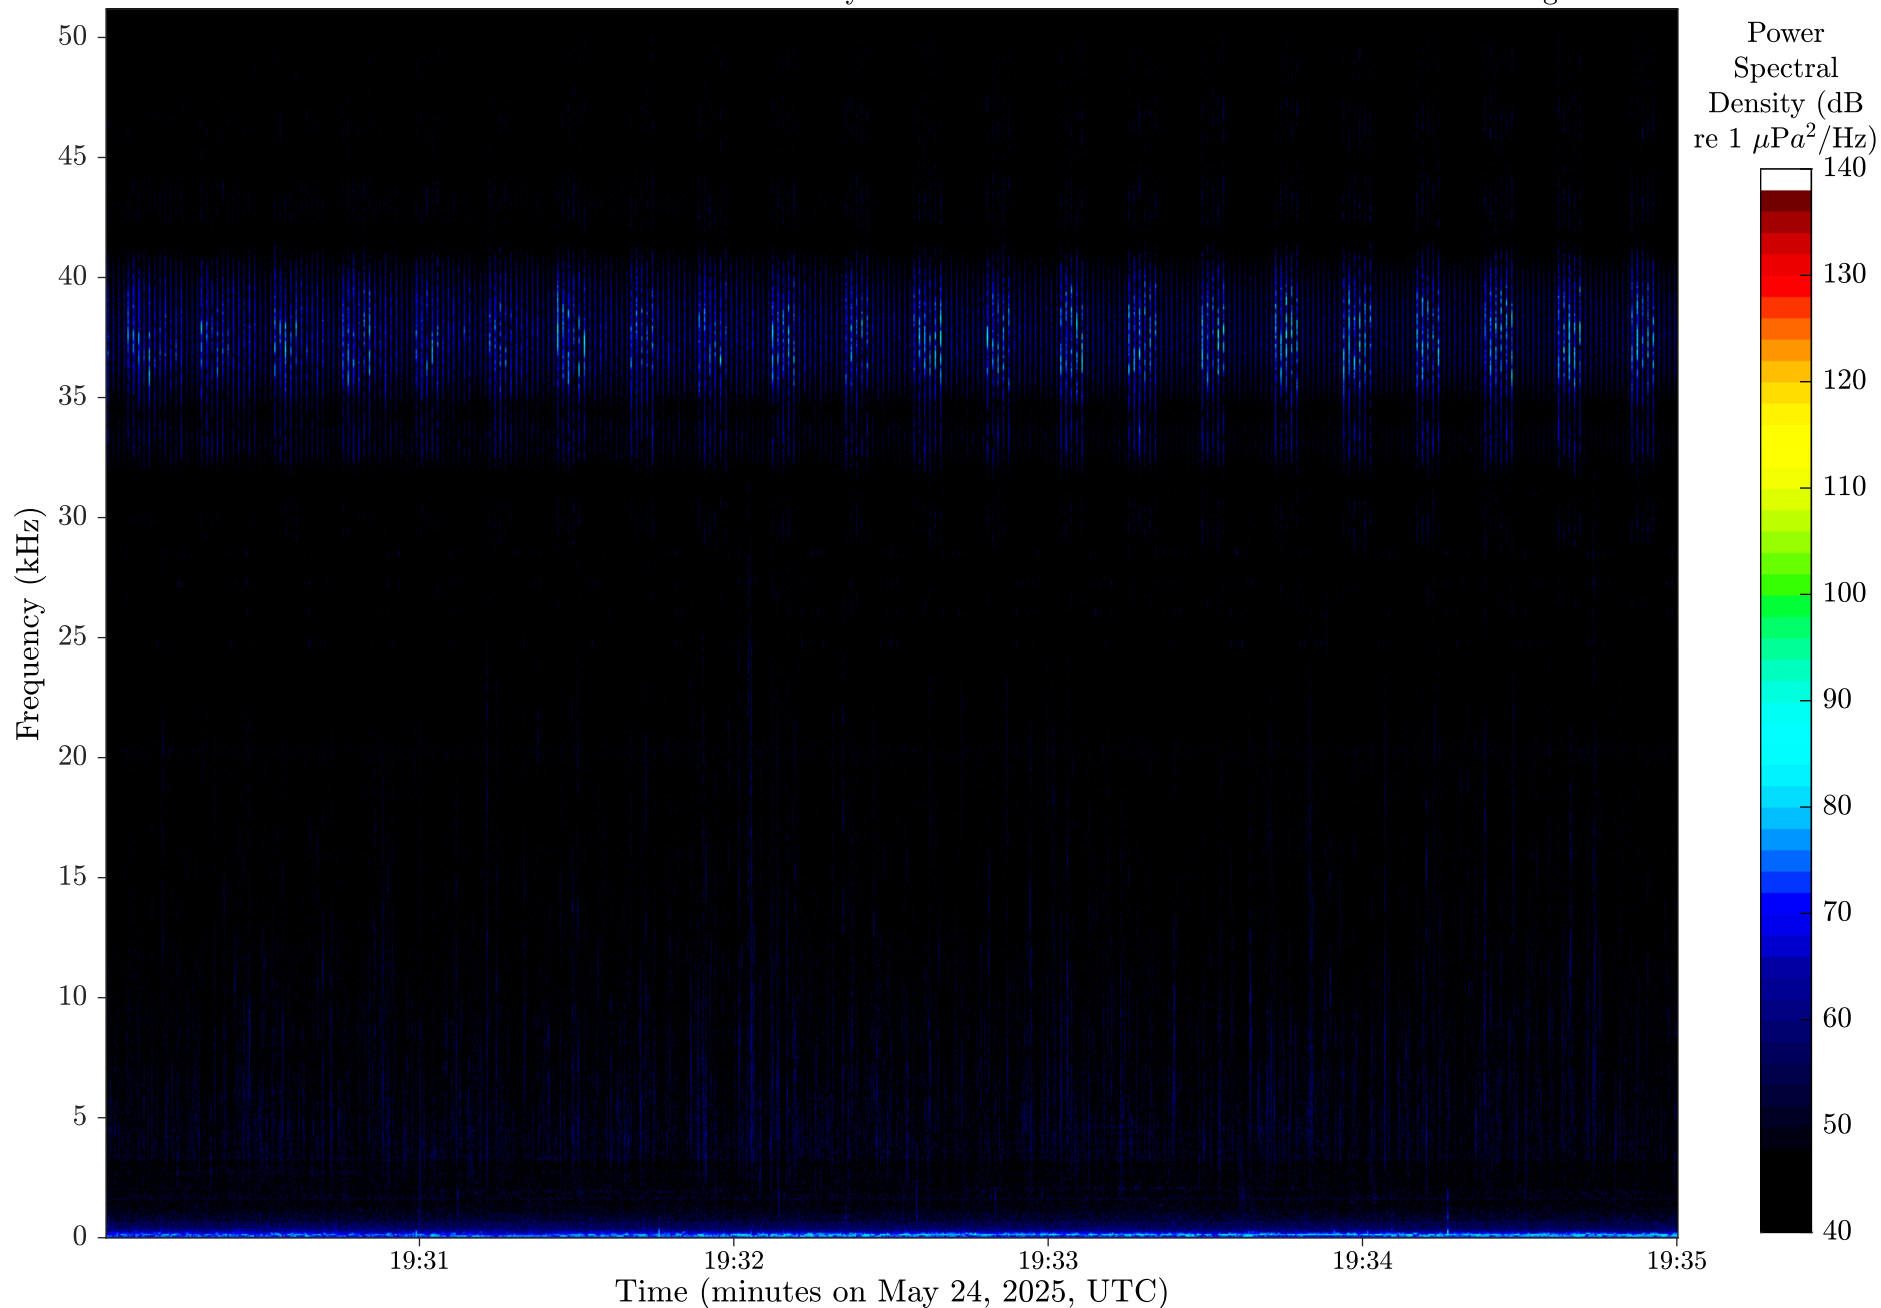


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:39 UTC

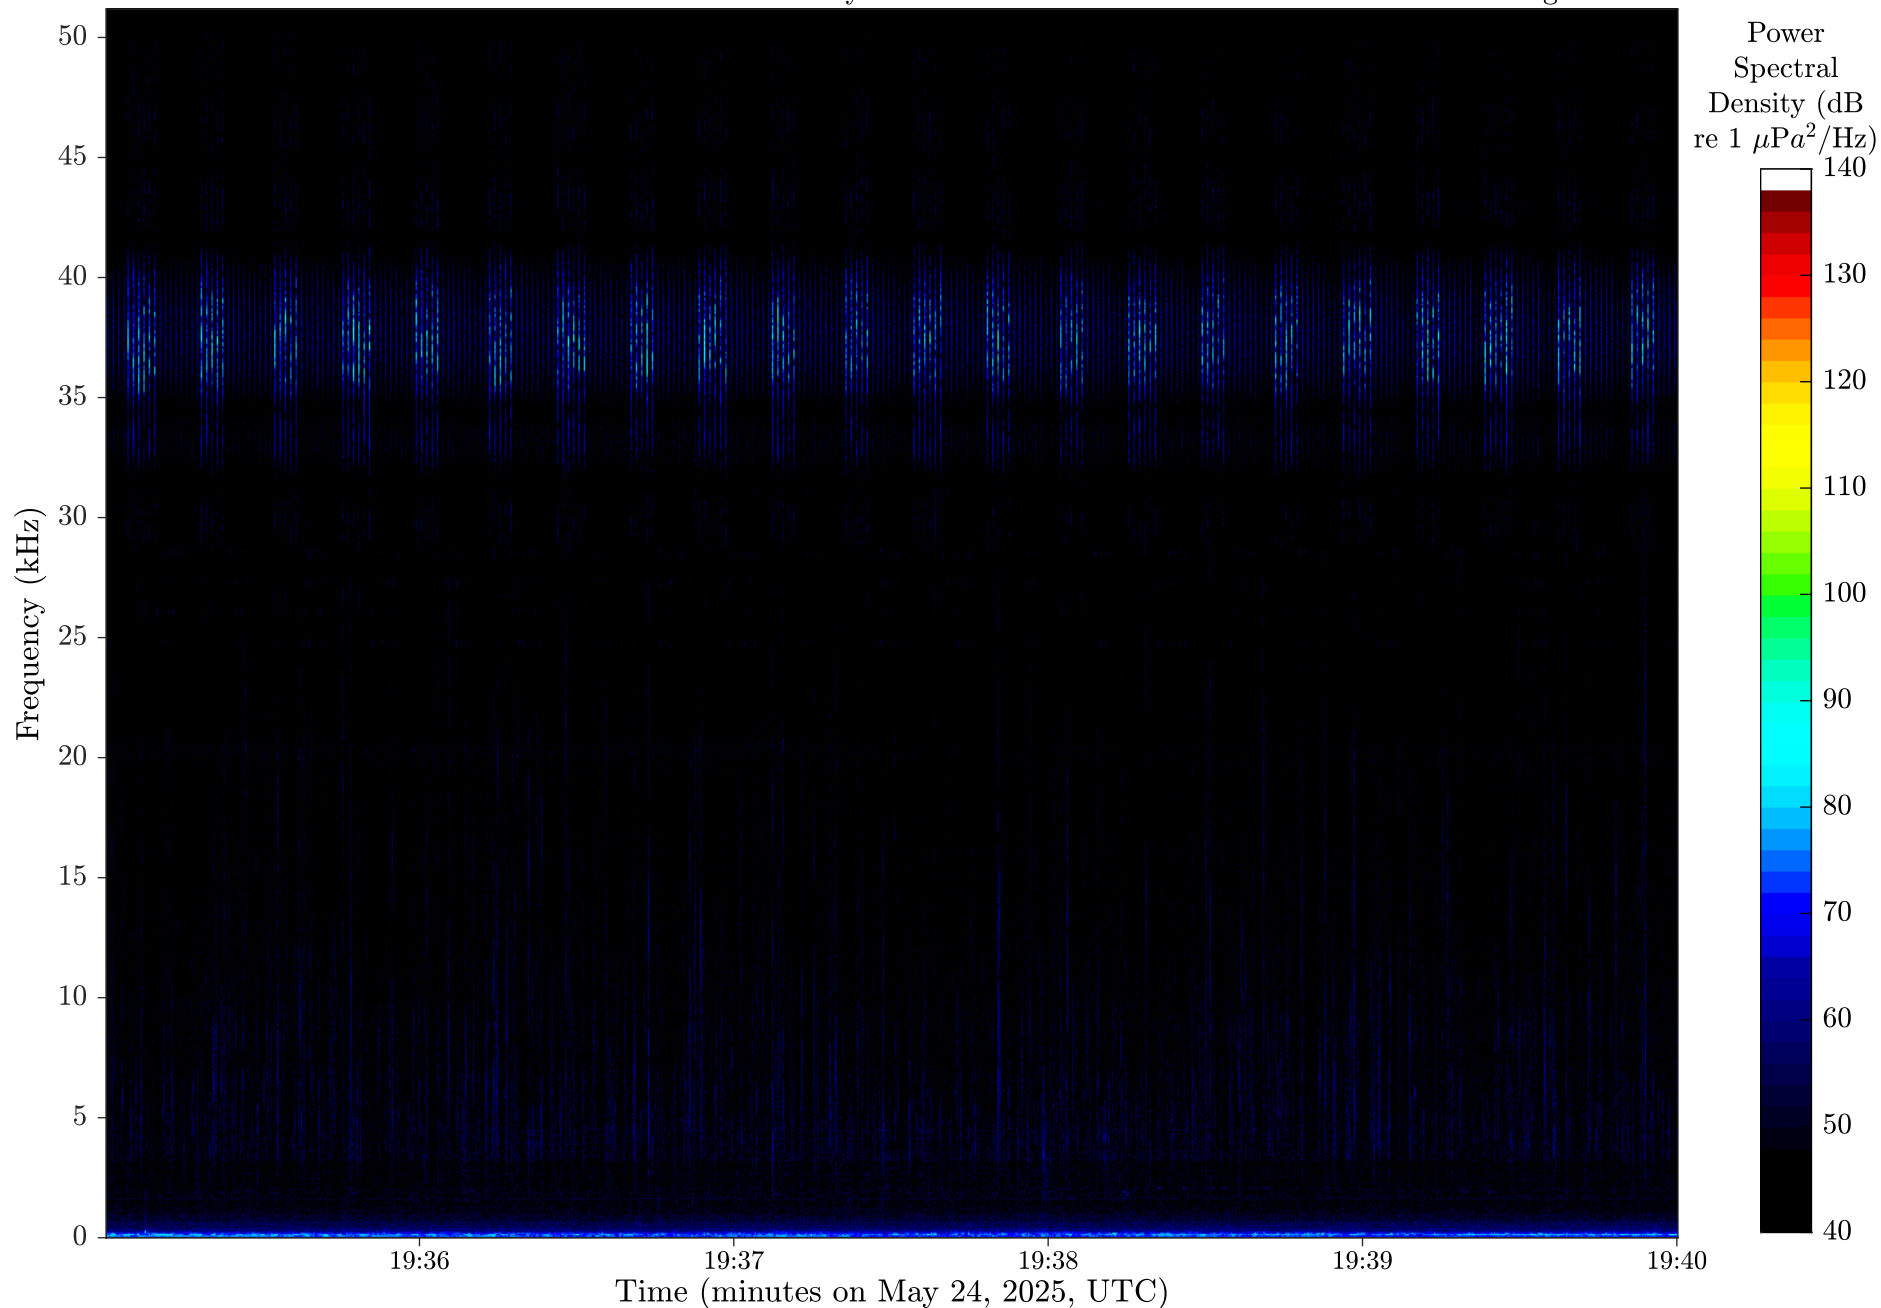


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:46 UTC

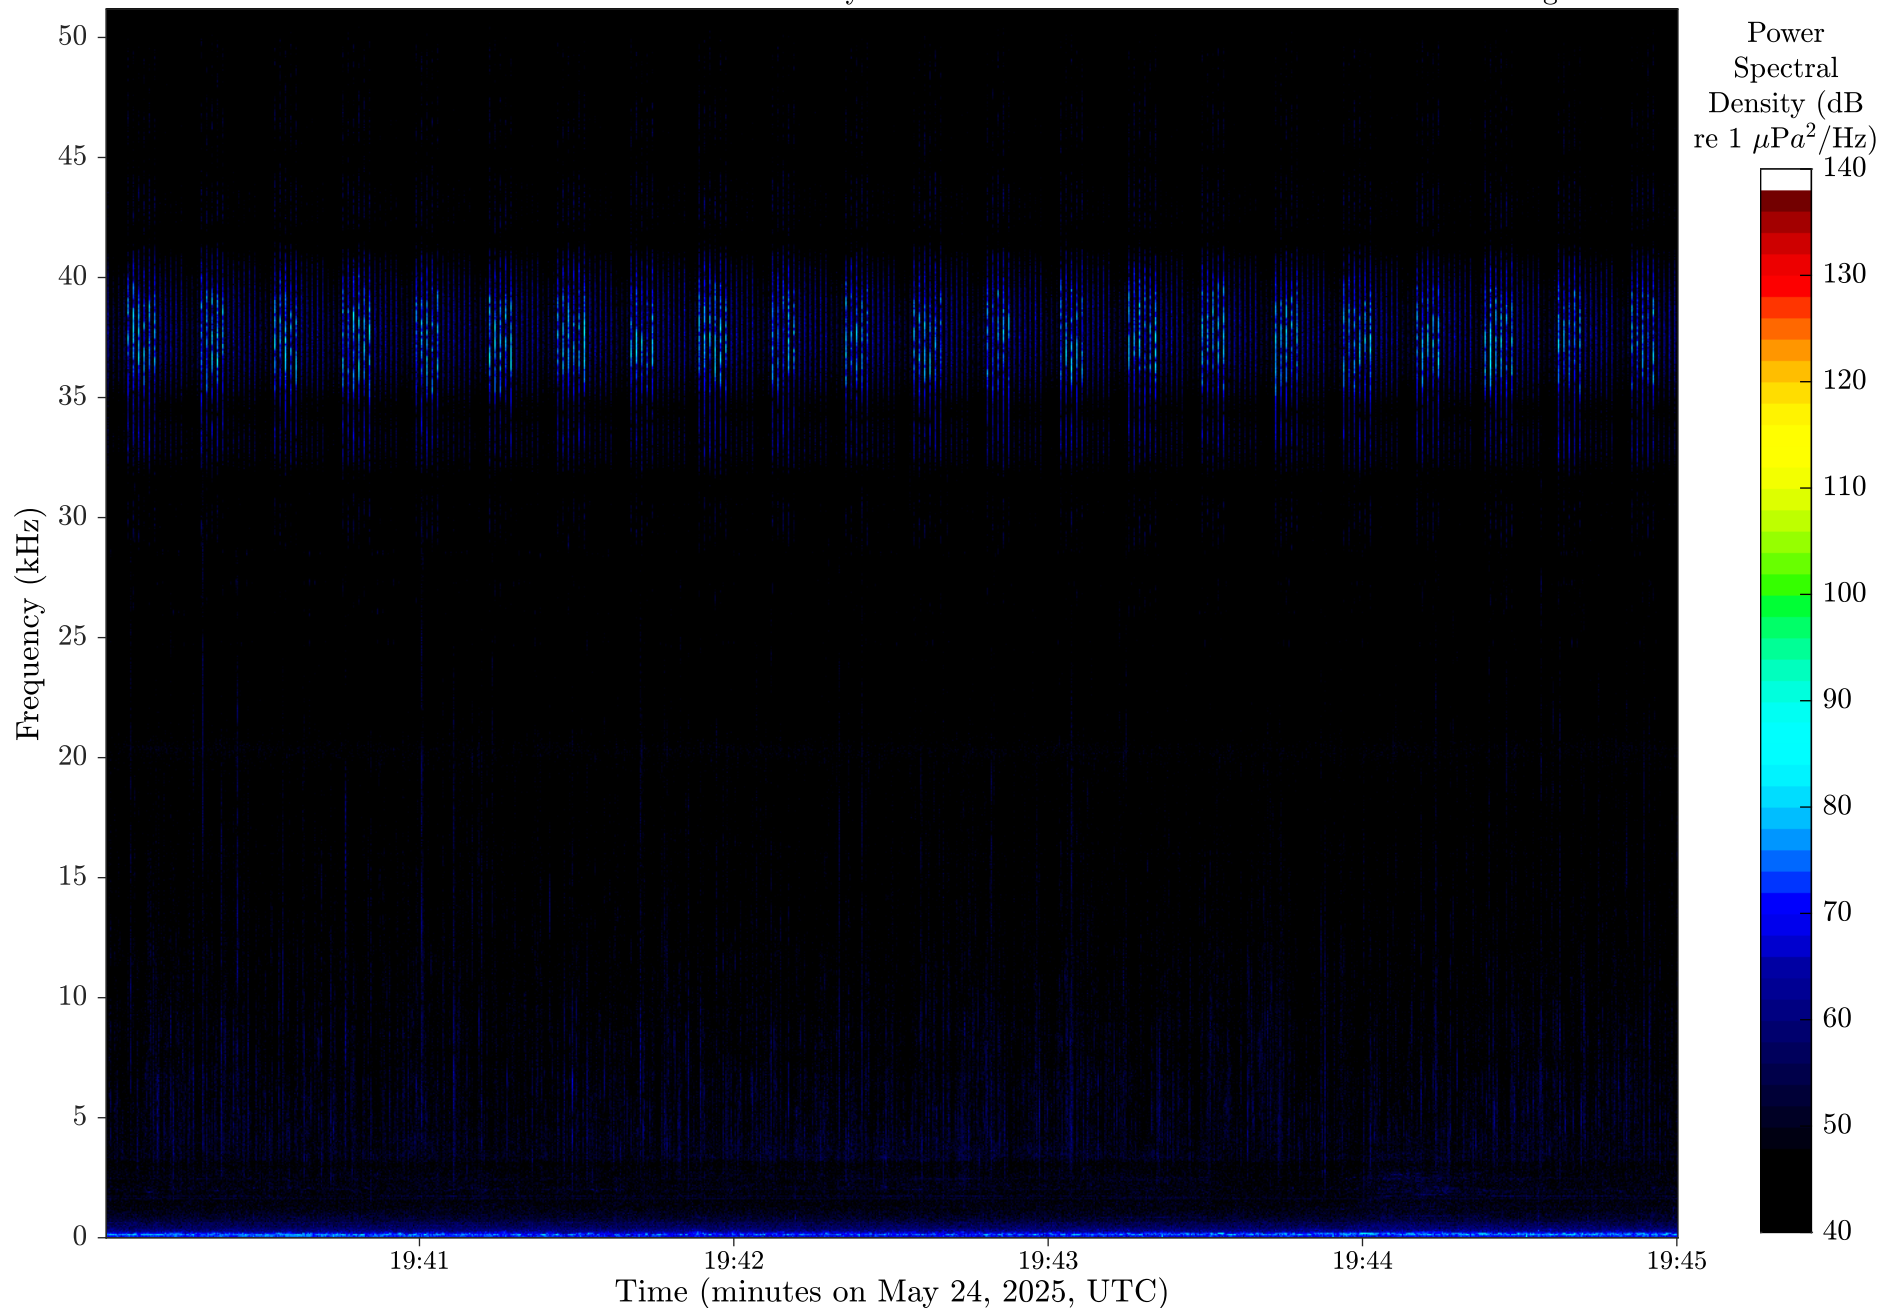


Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:52 UTC

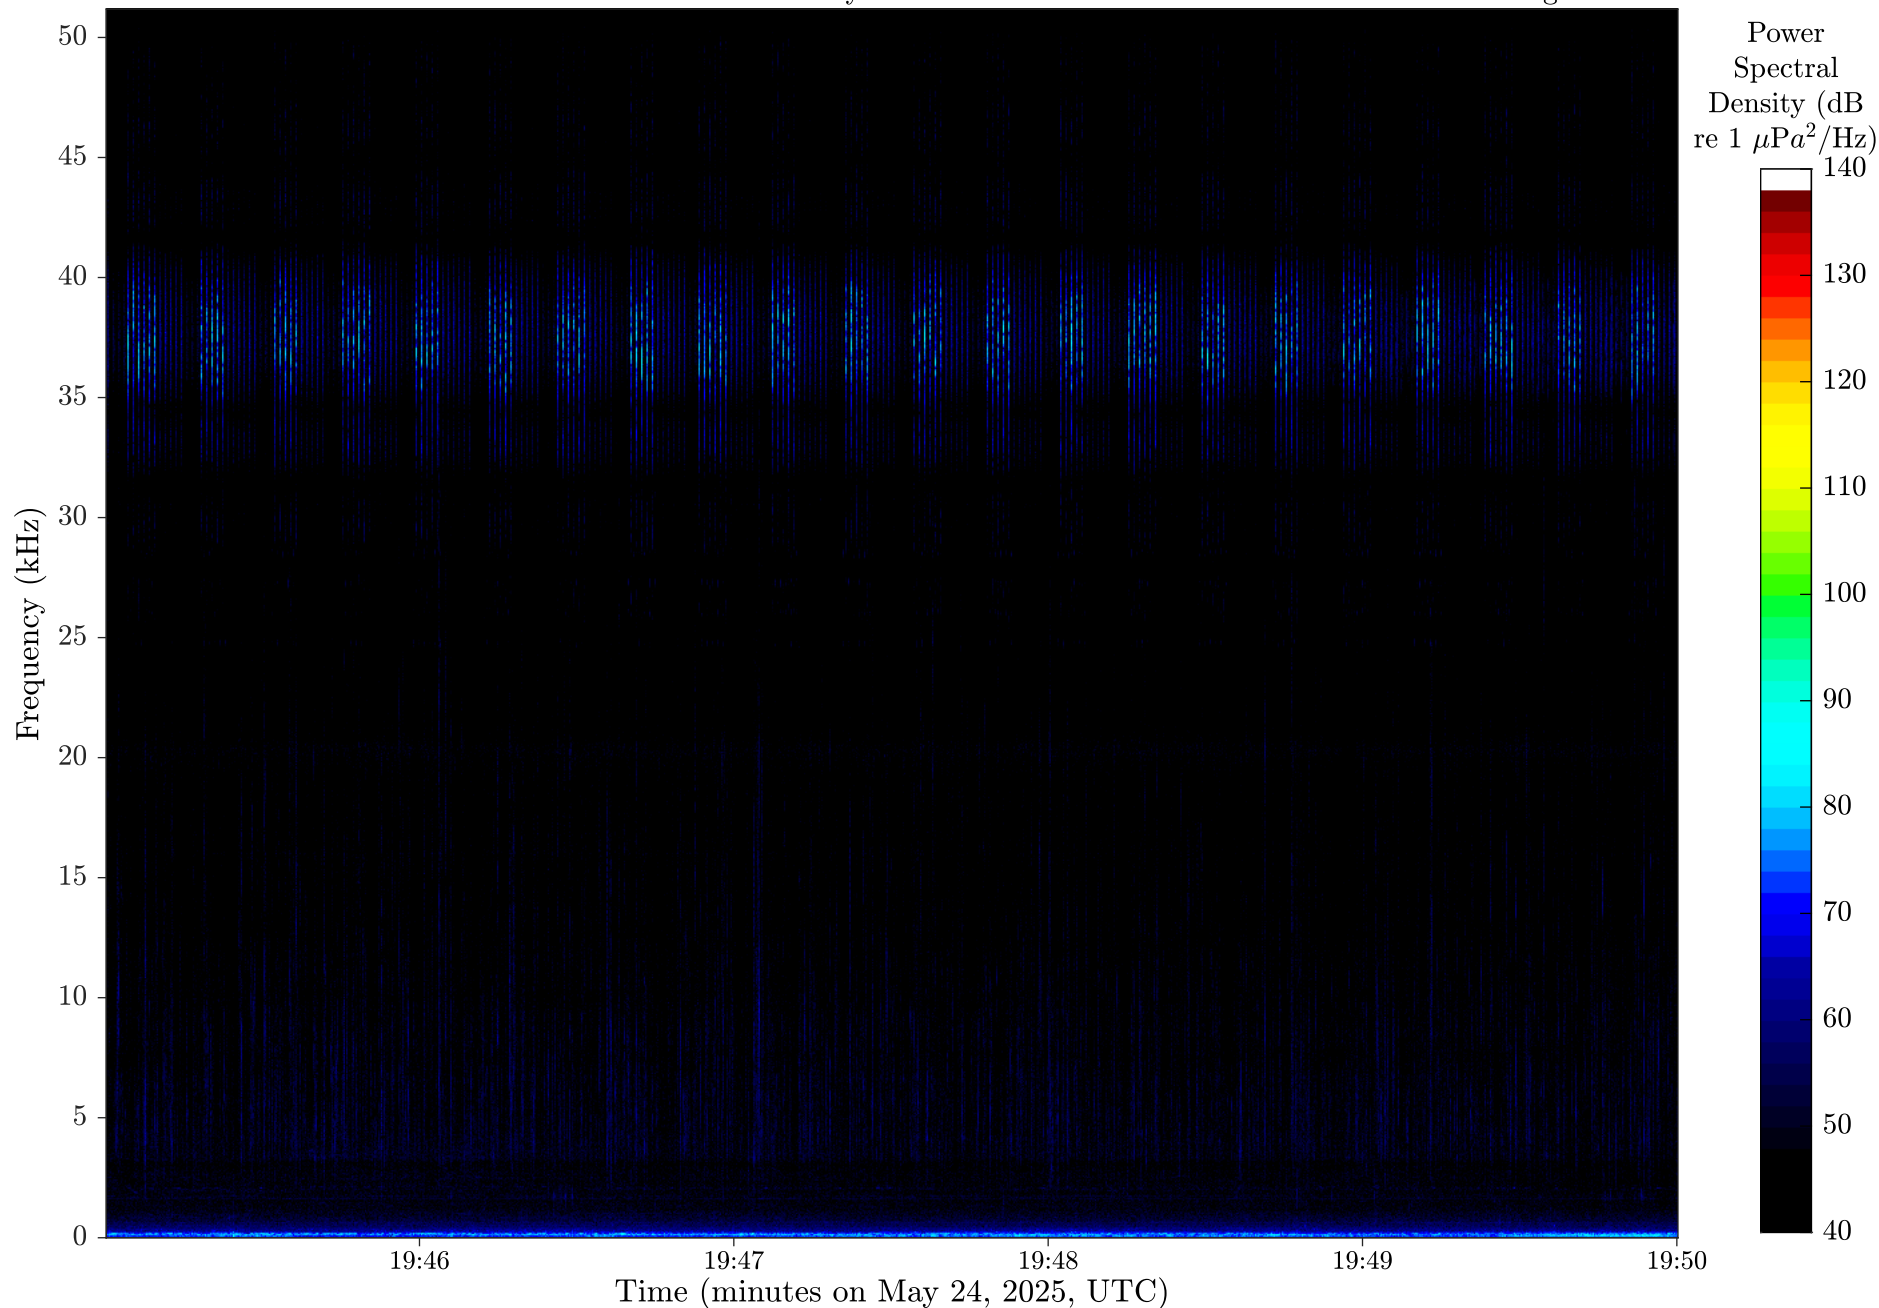


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:00 UTC

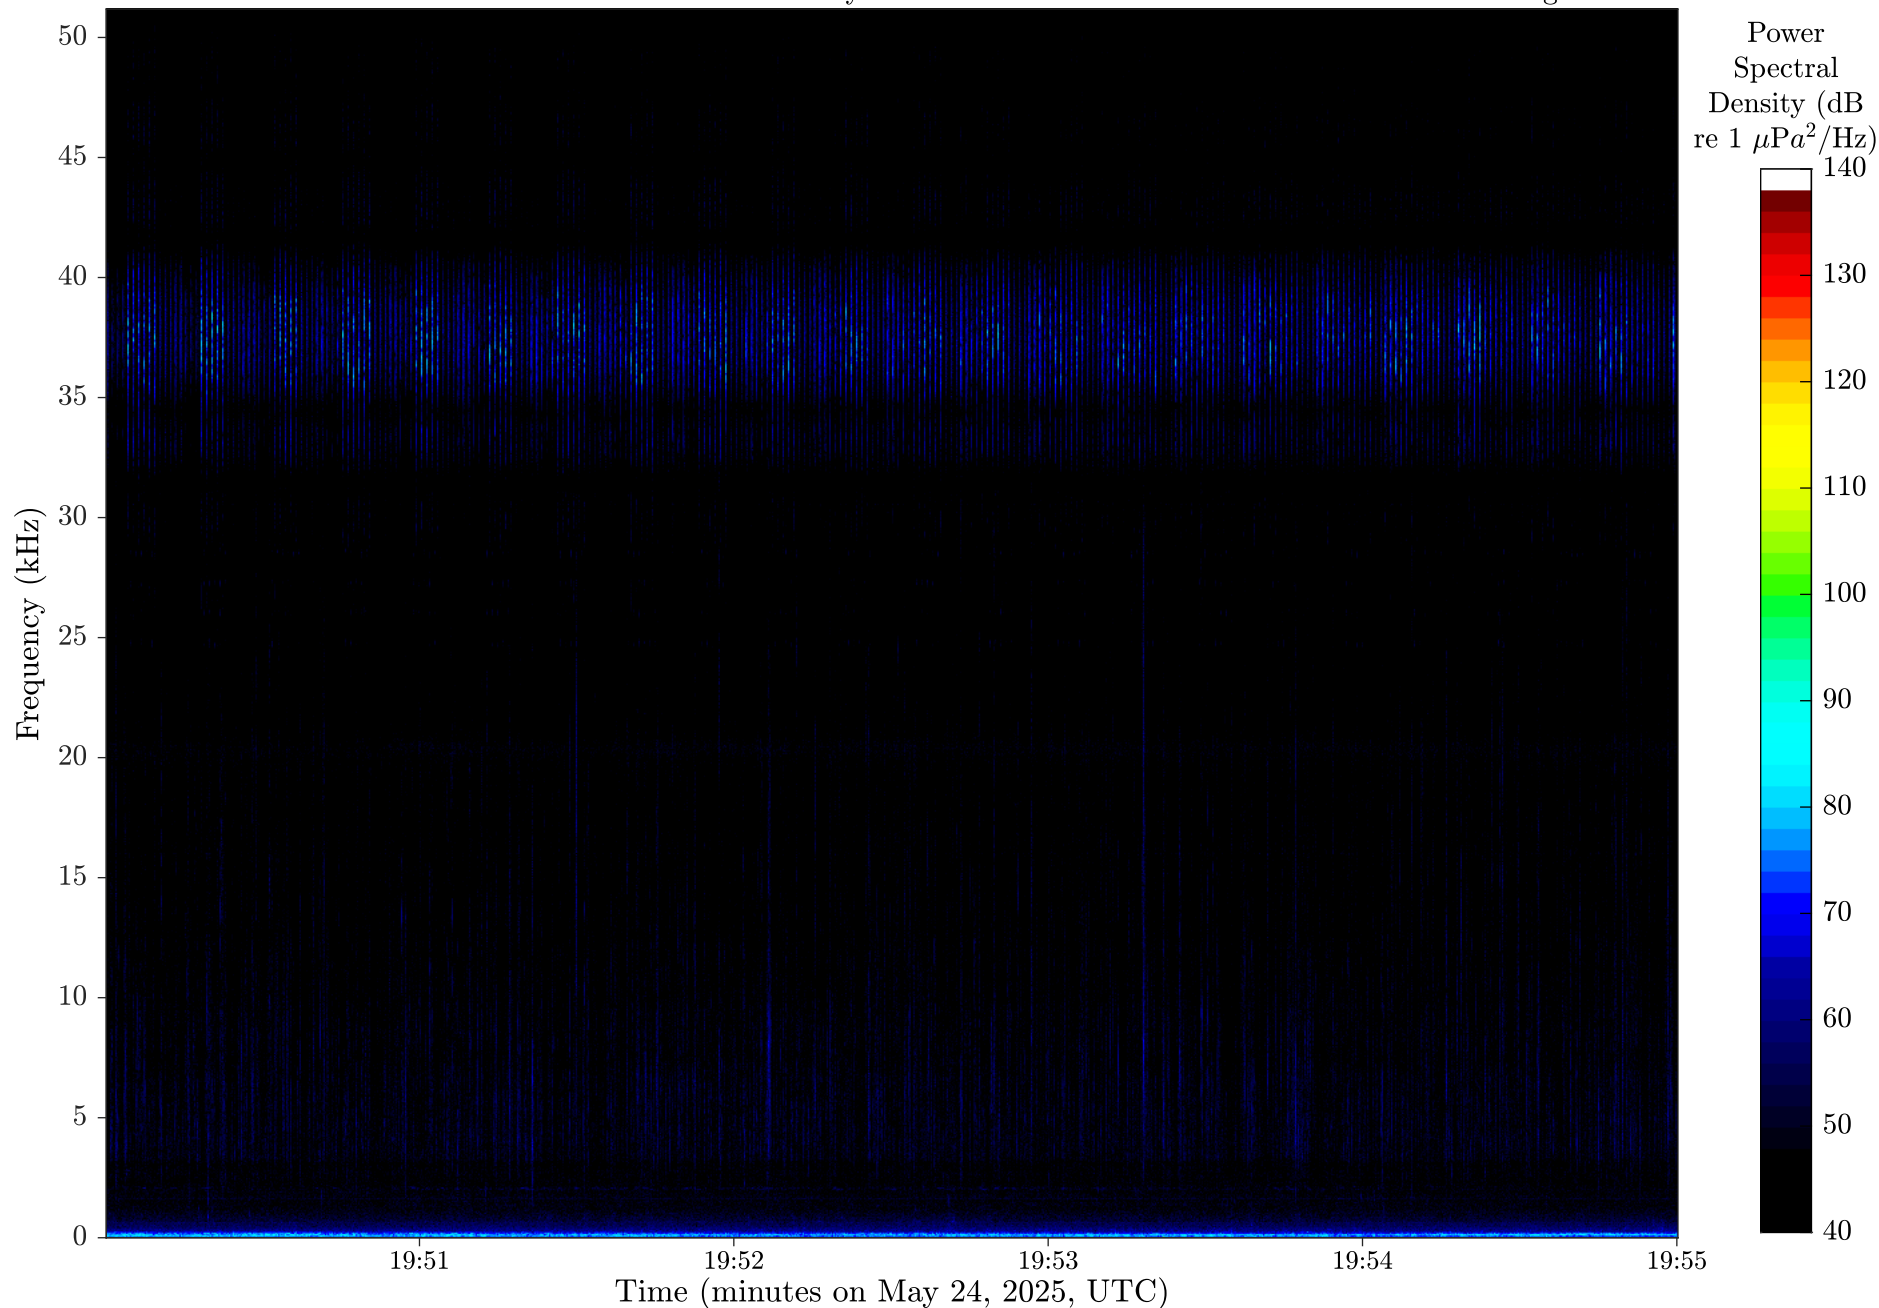


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:07 UTC

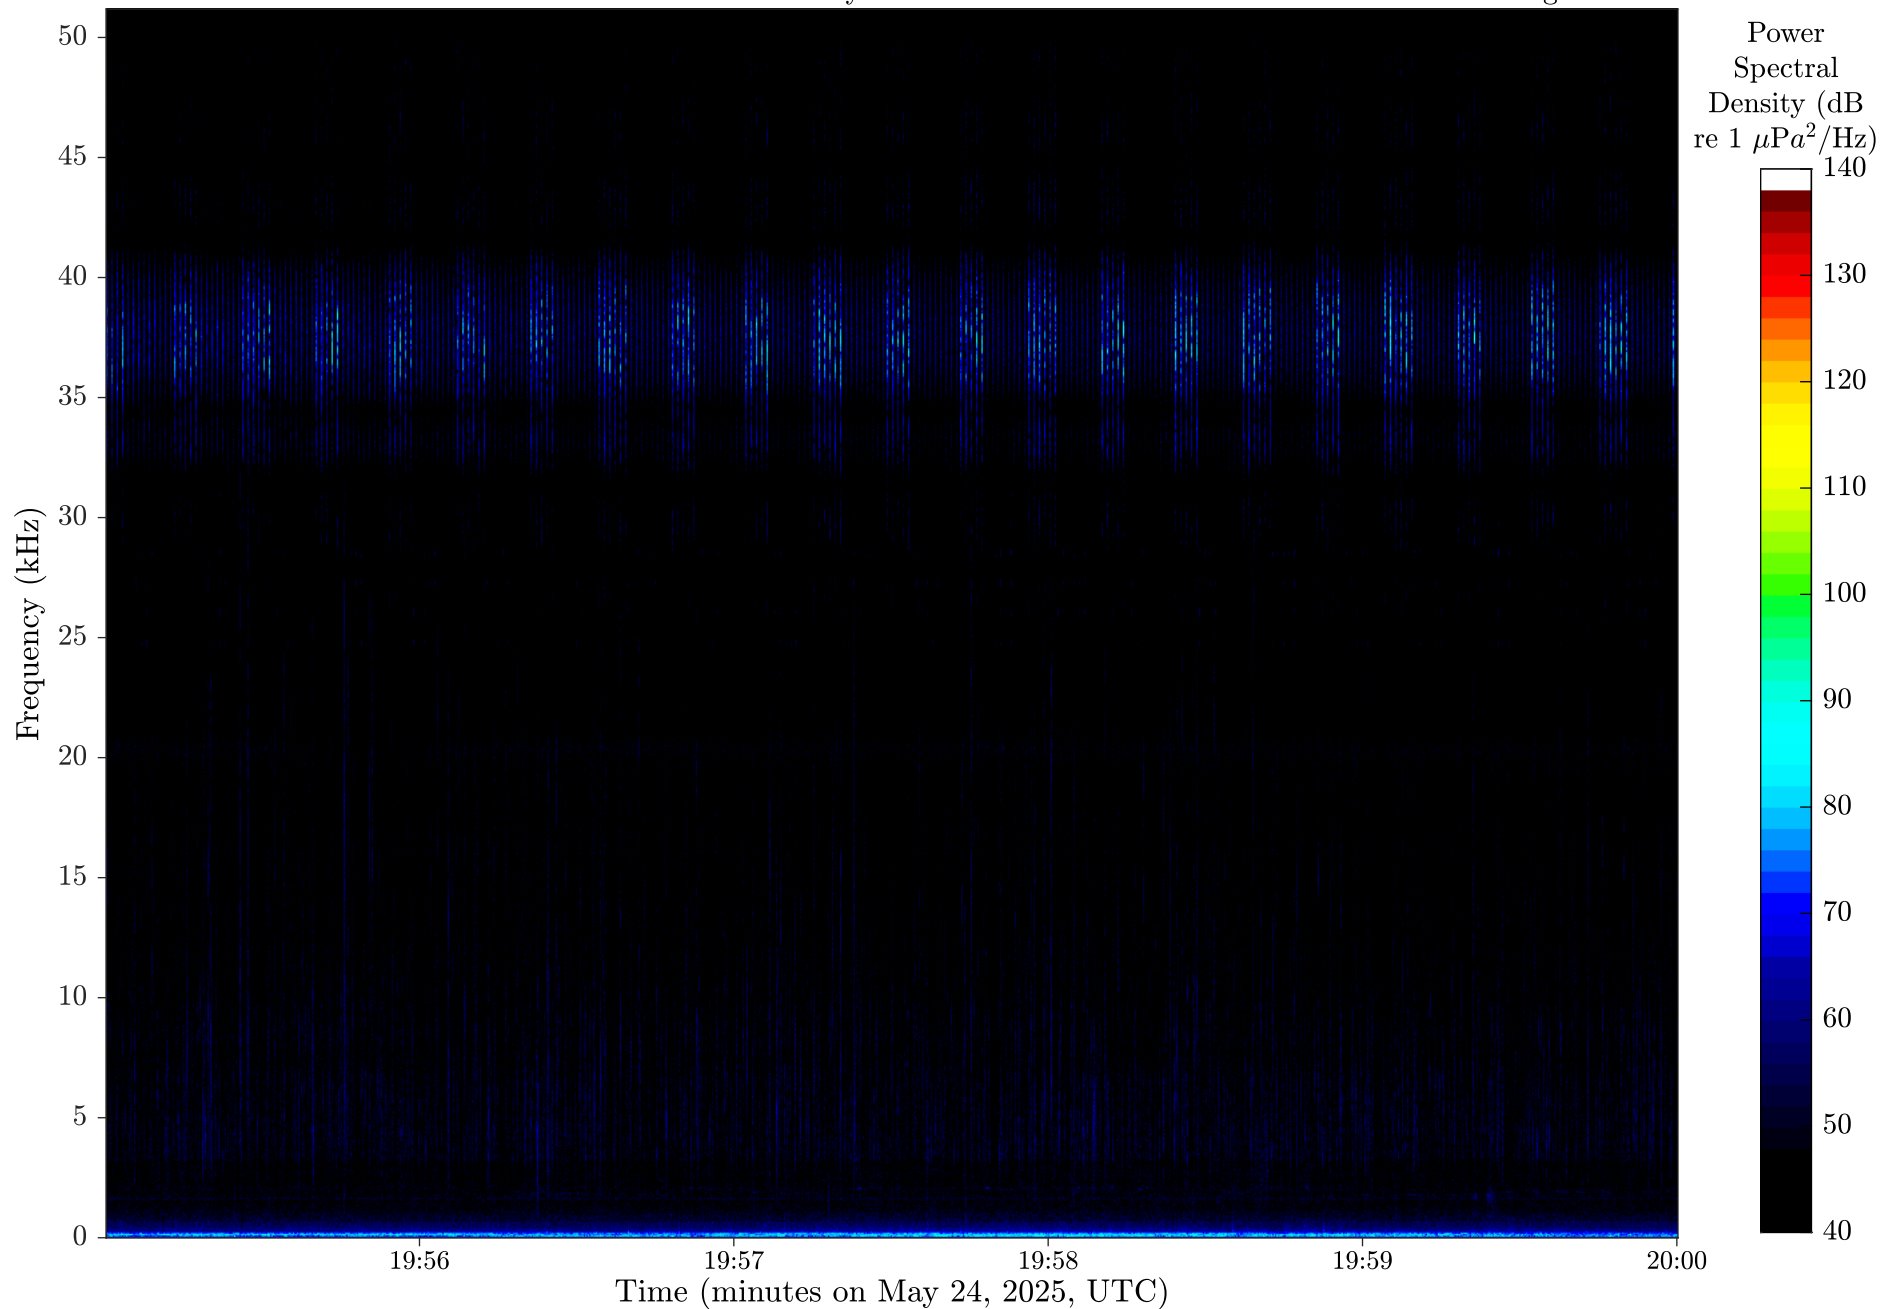


Comments: 34.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:14 UTC

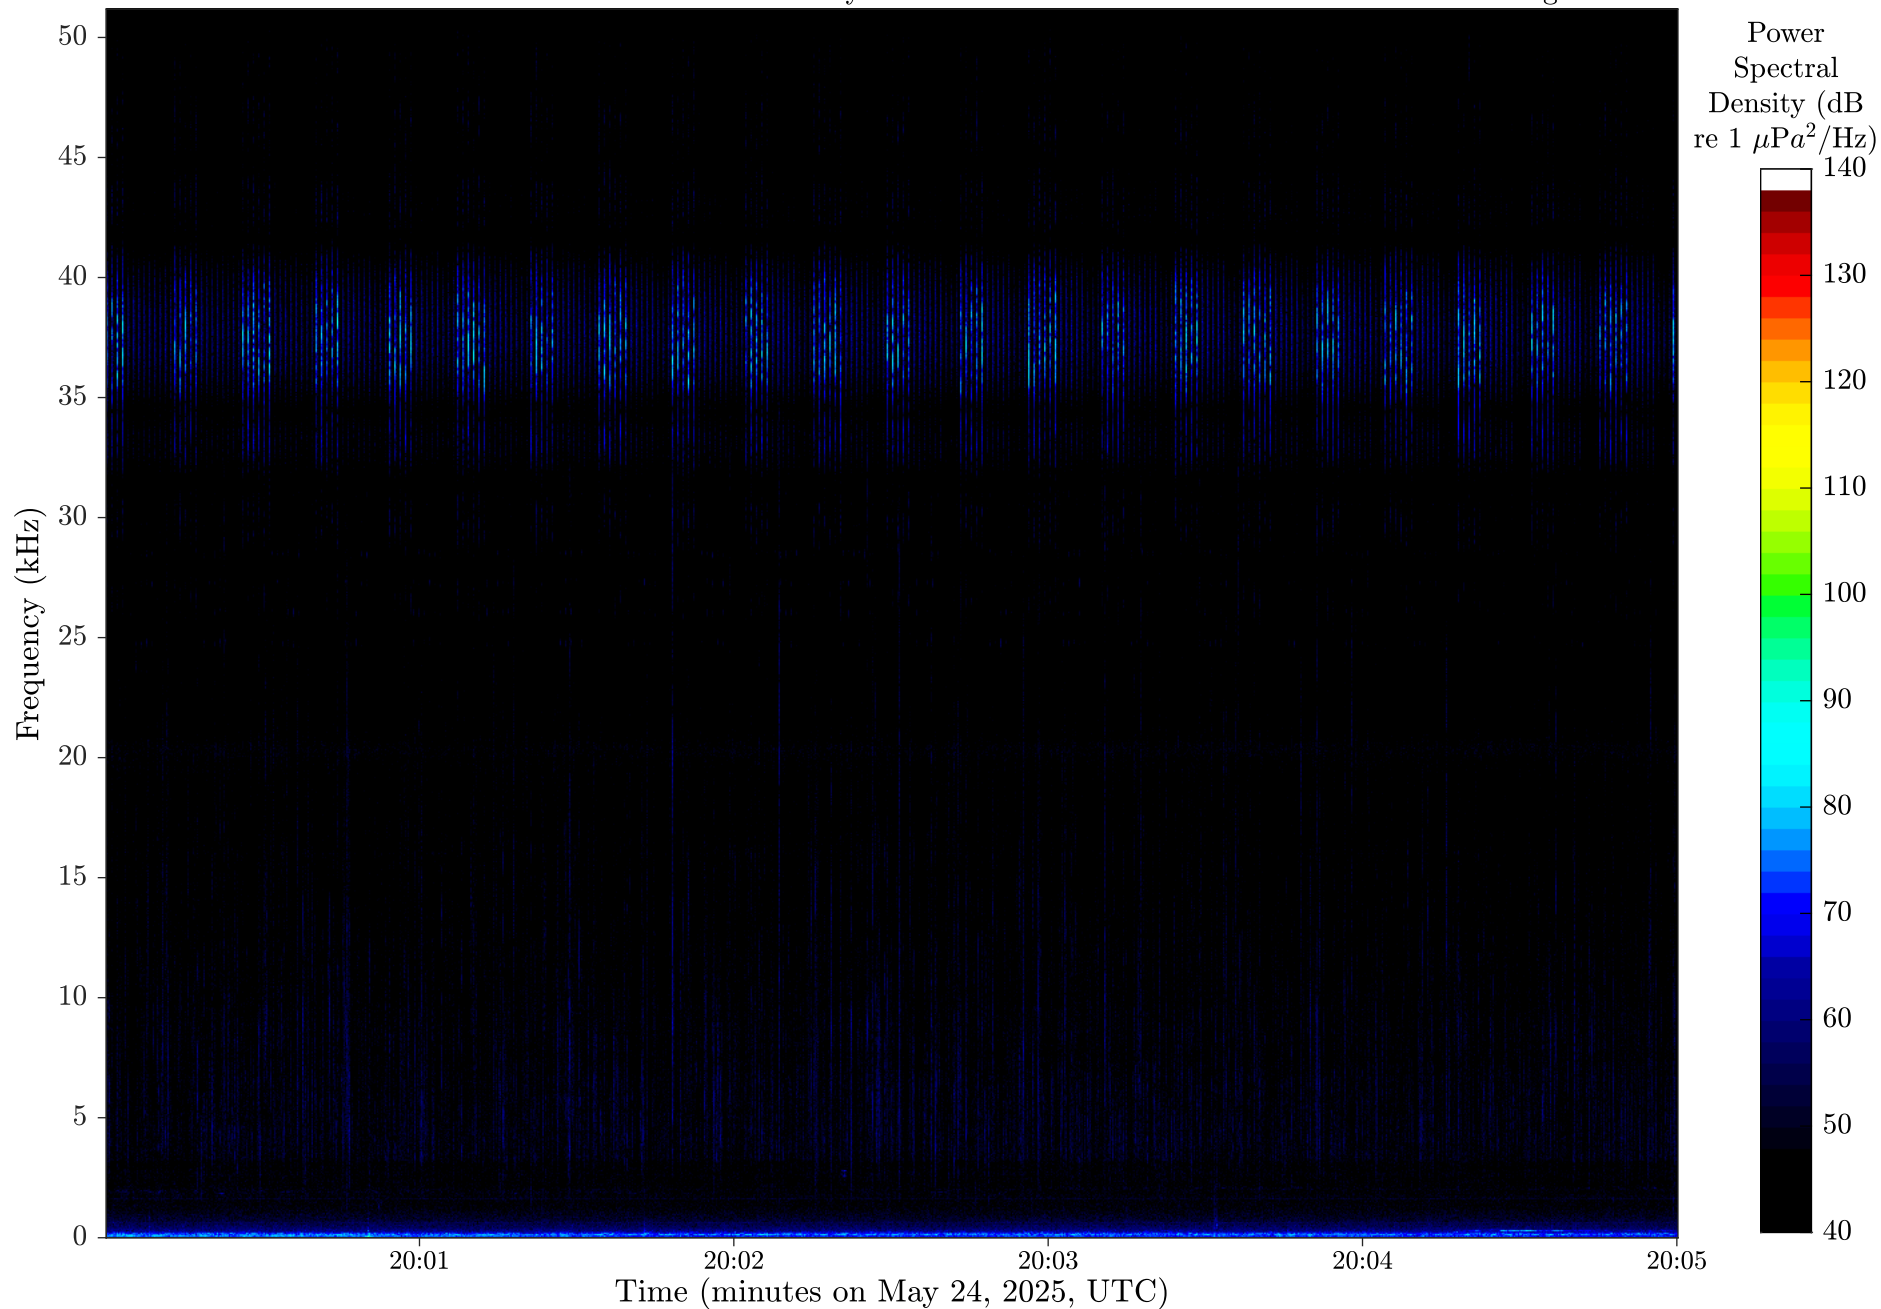


Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:21 UTC

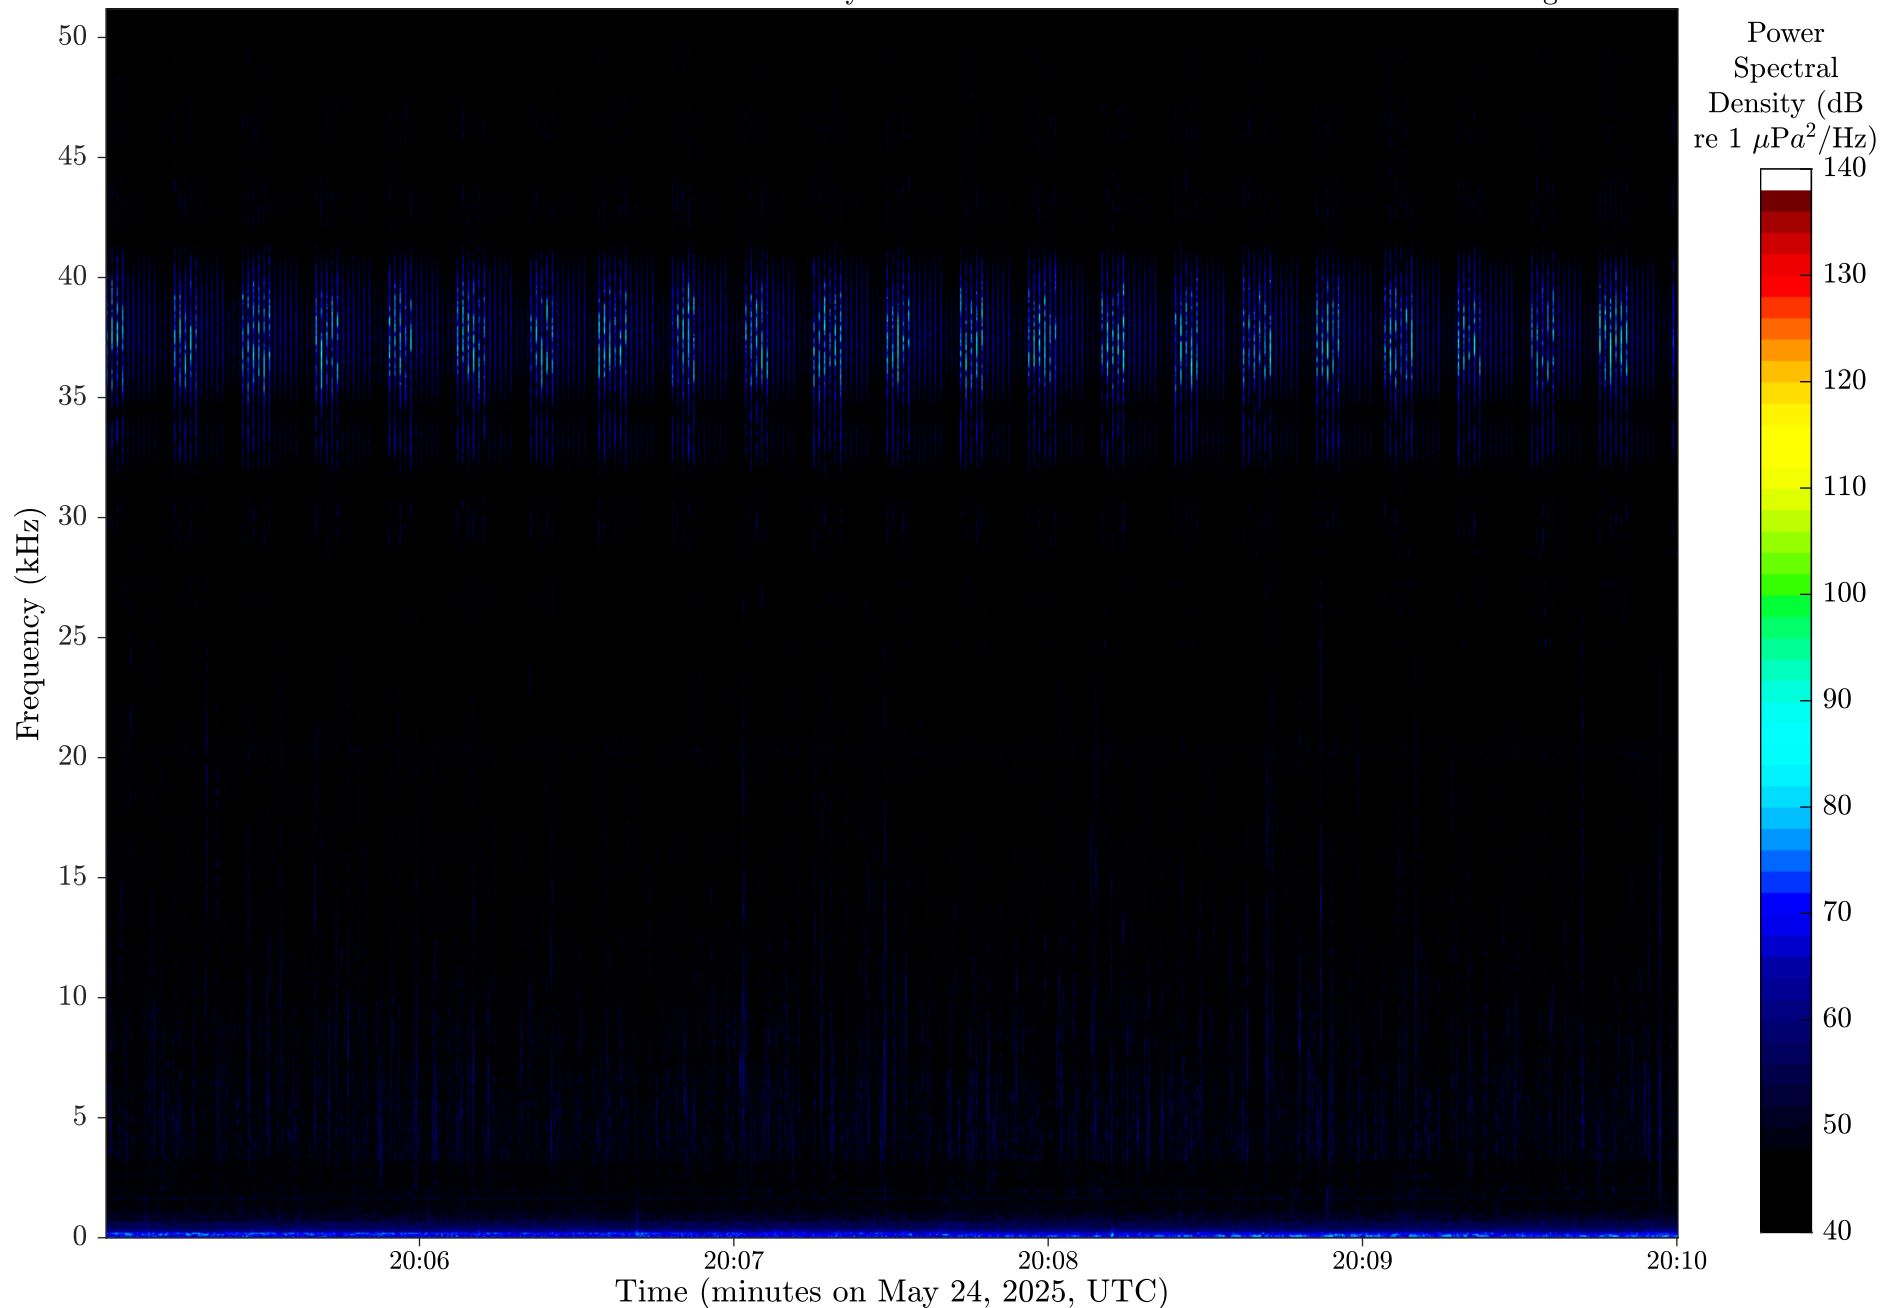


Comments: 35.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:41:28 UTC

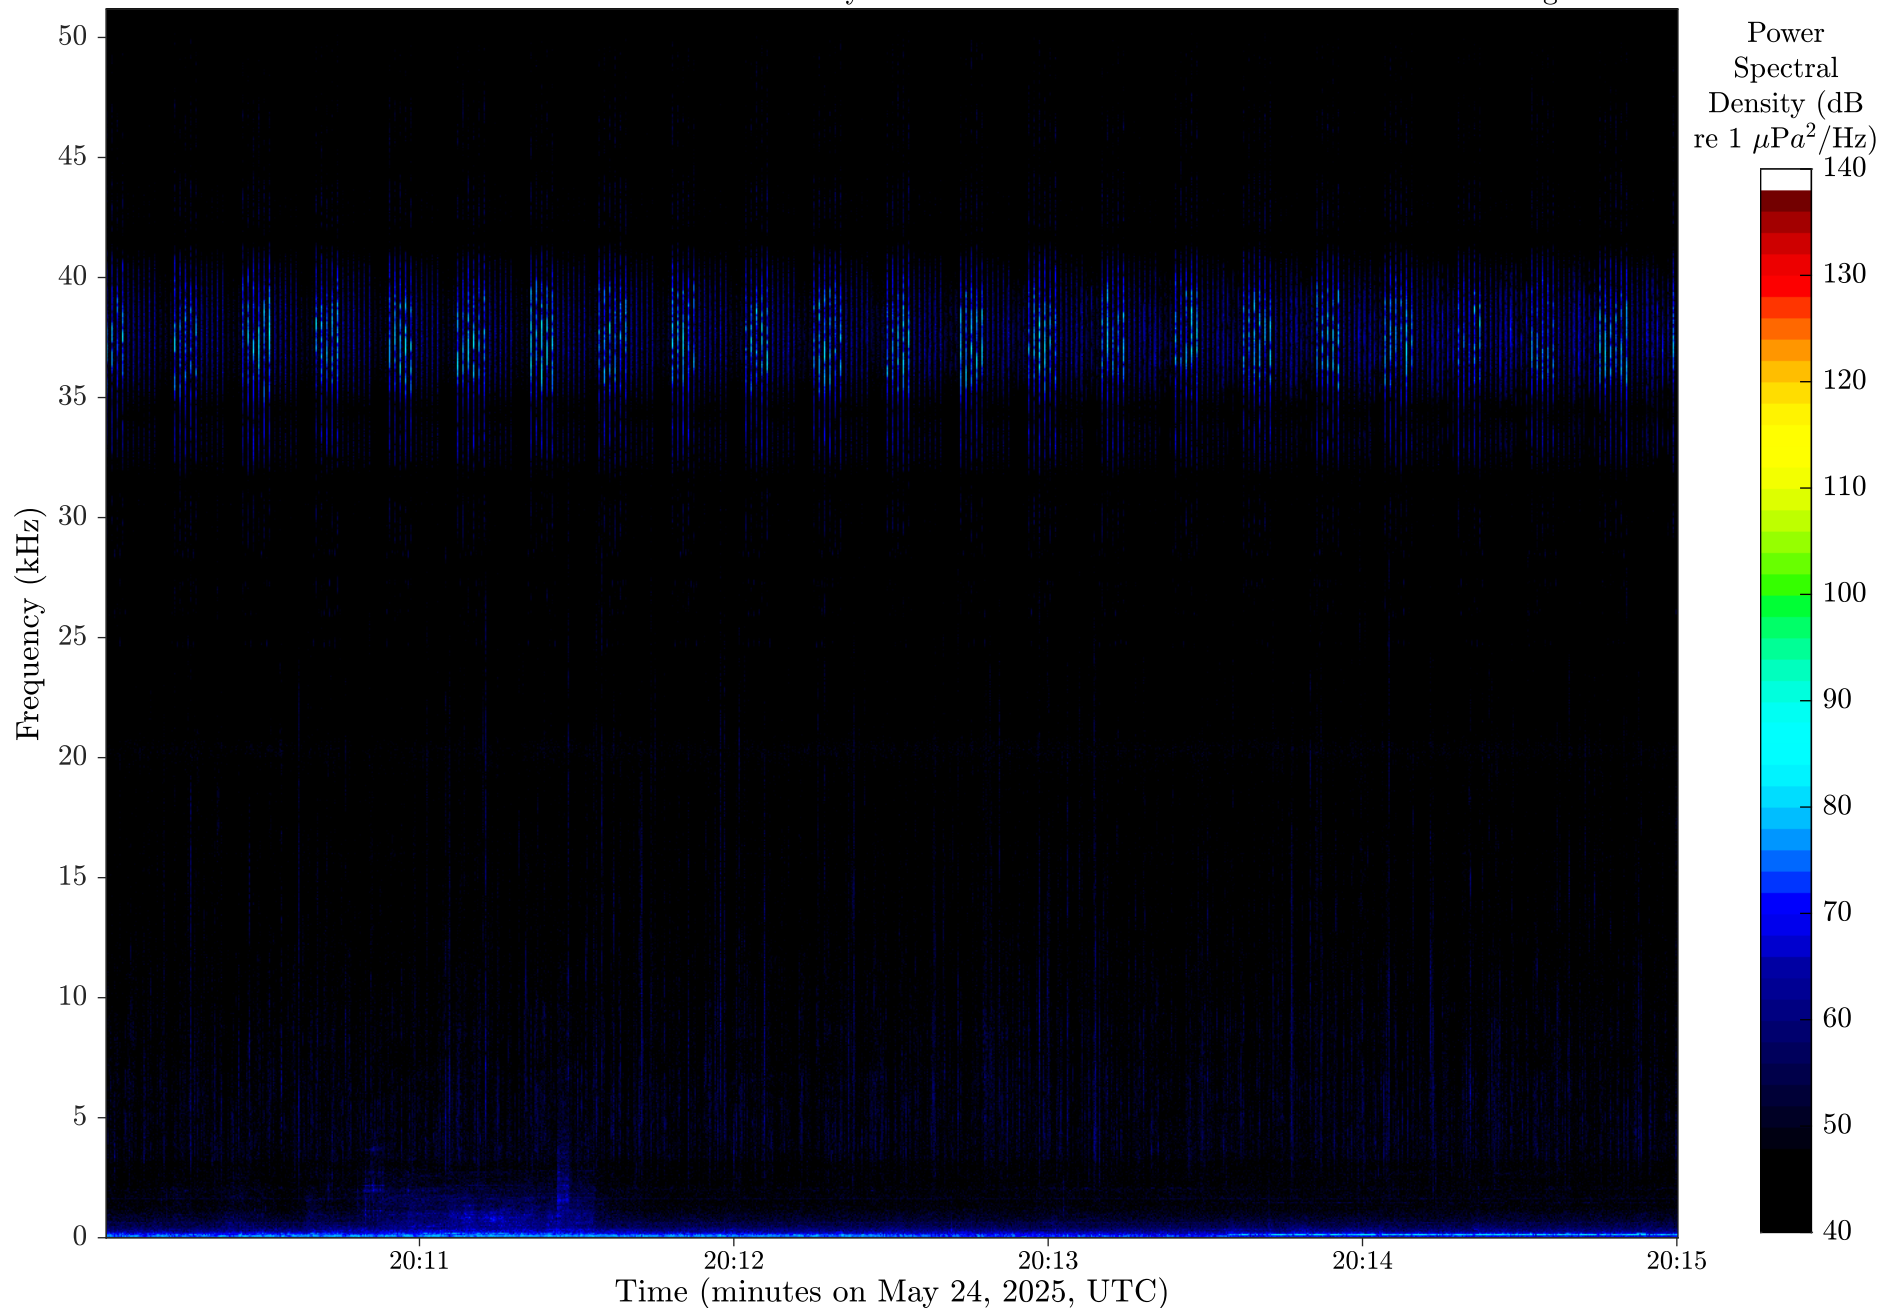

Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:41:36 UTC

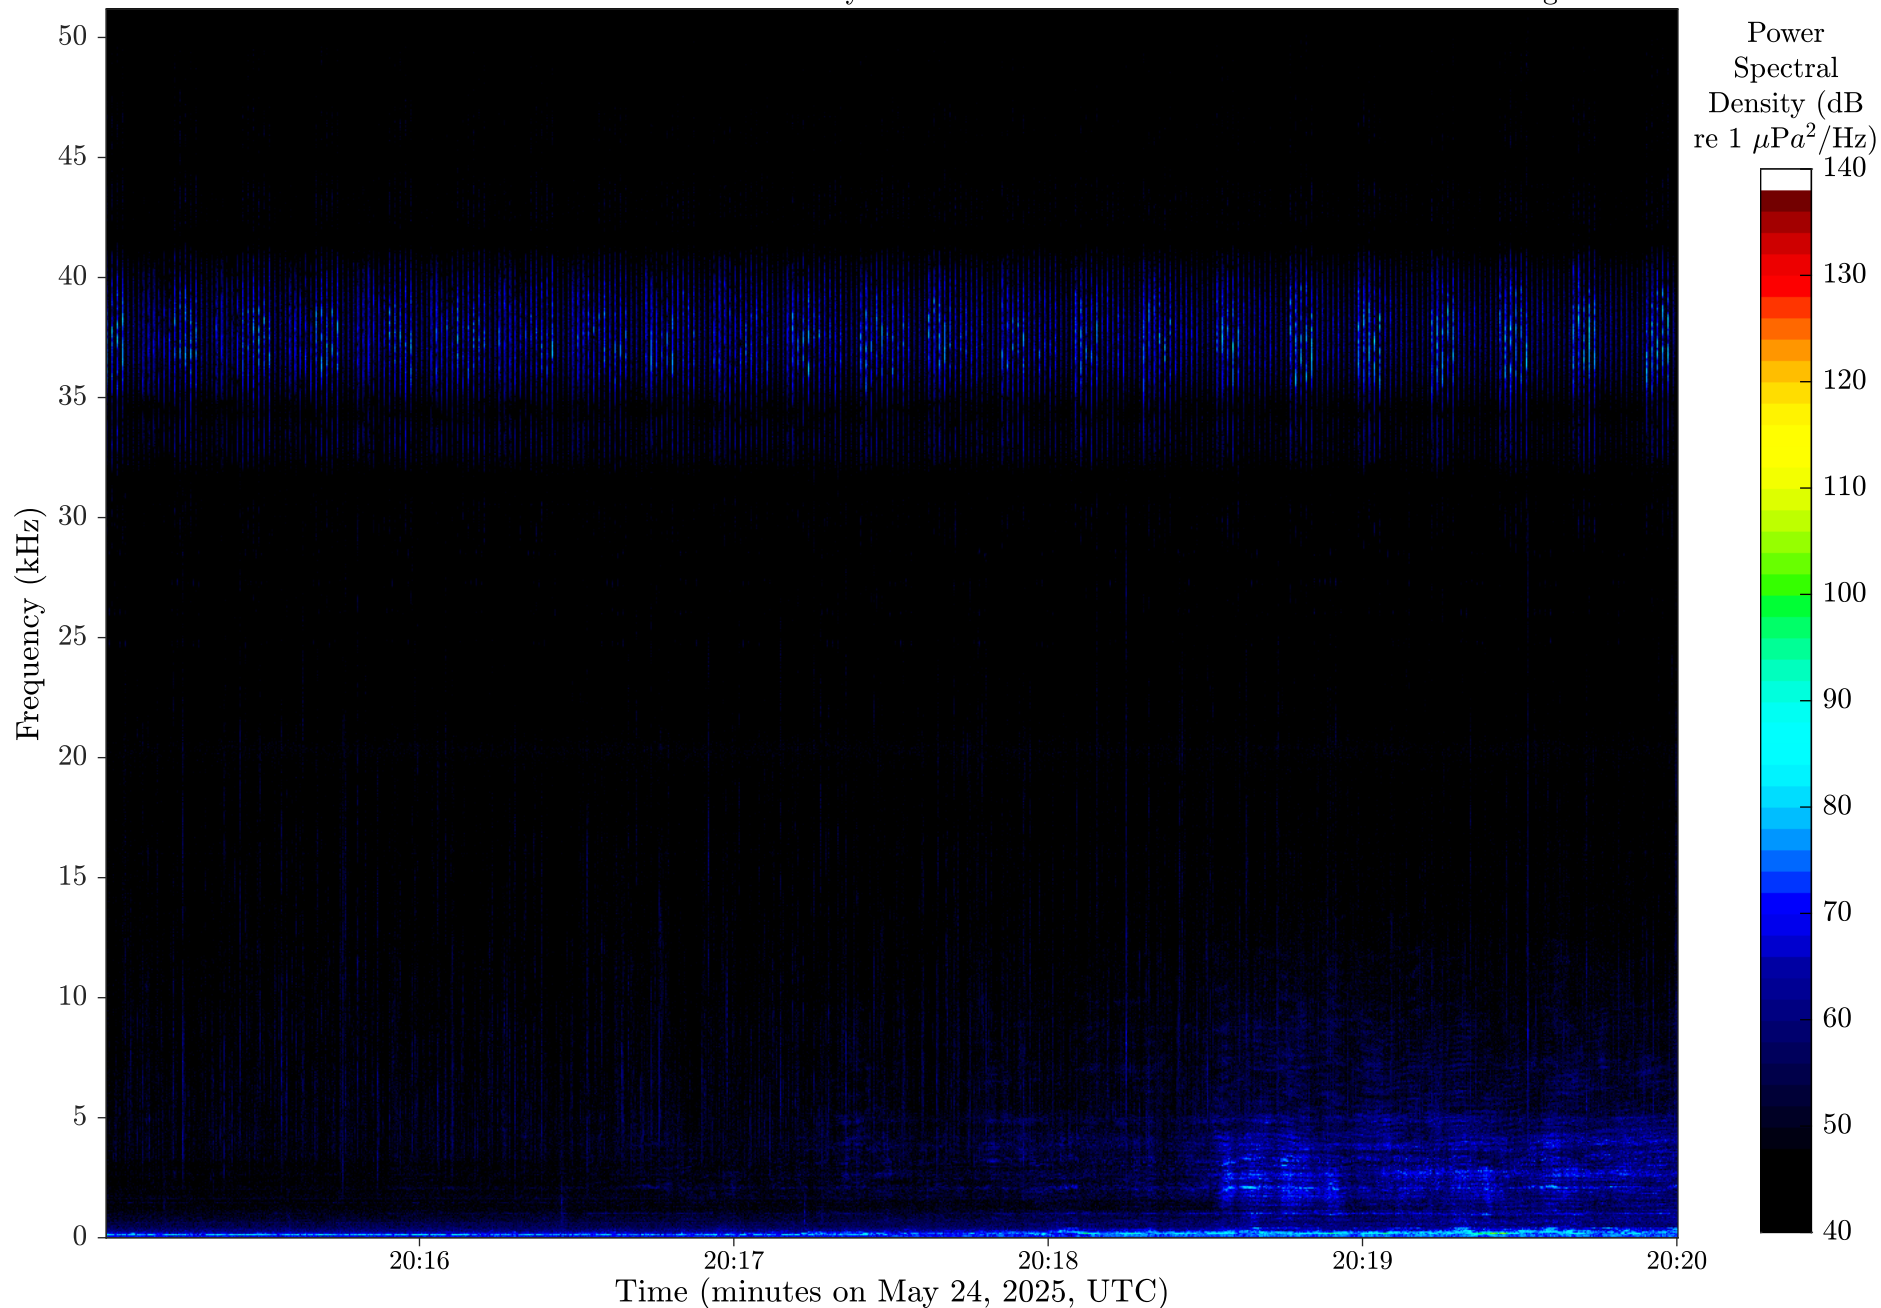

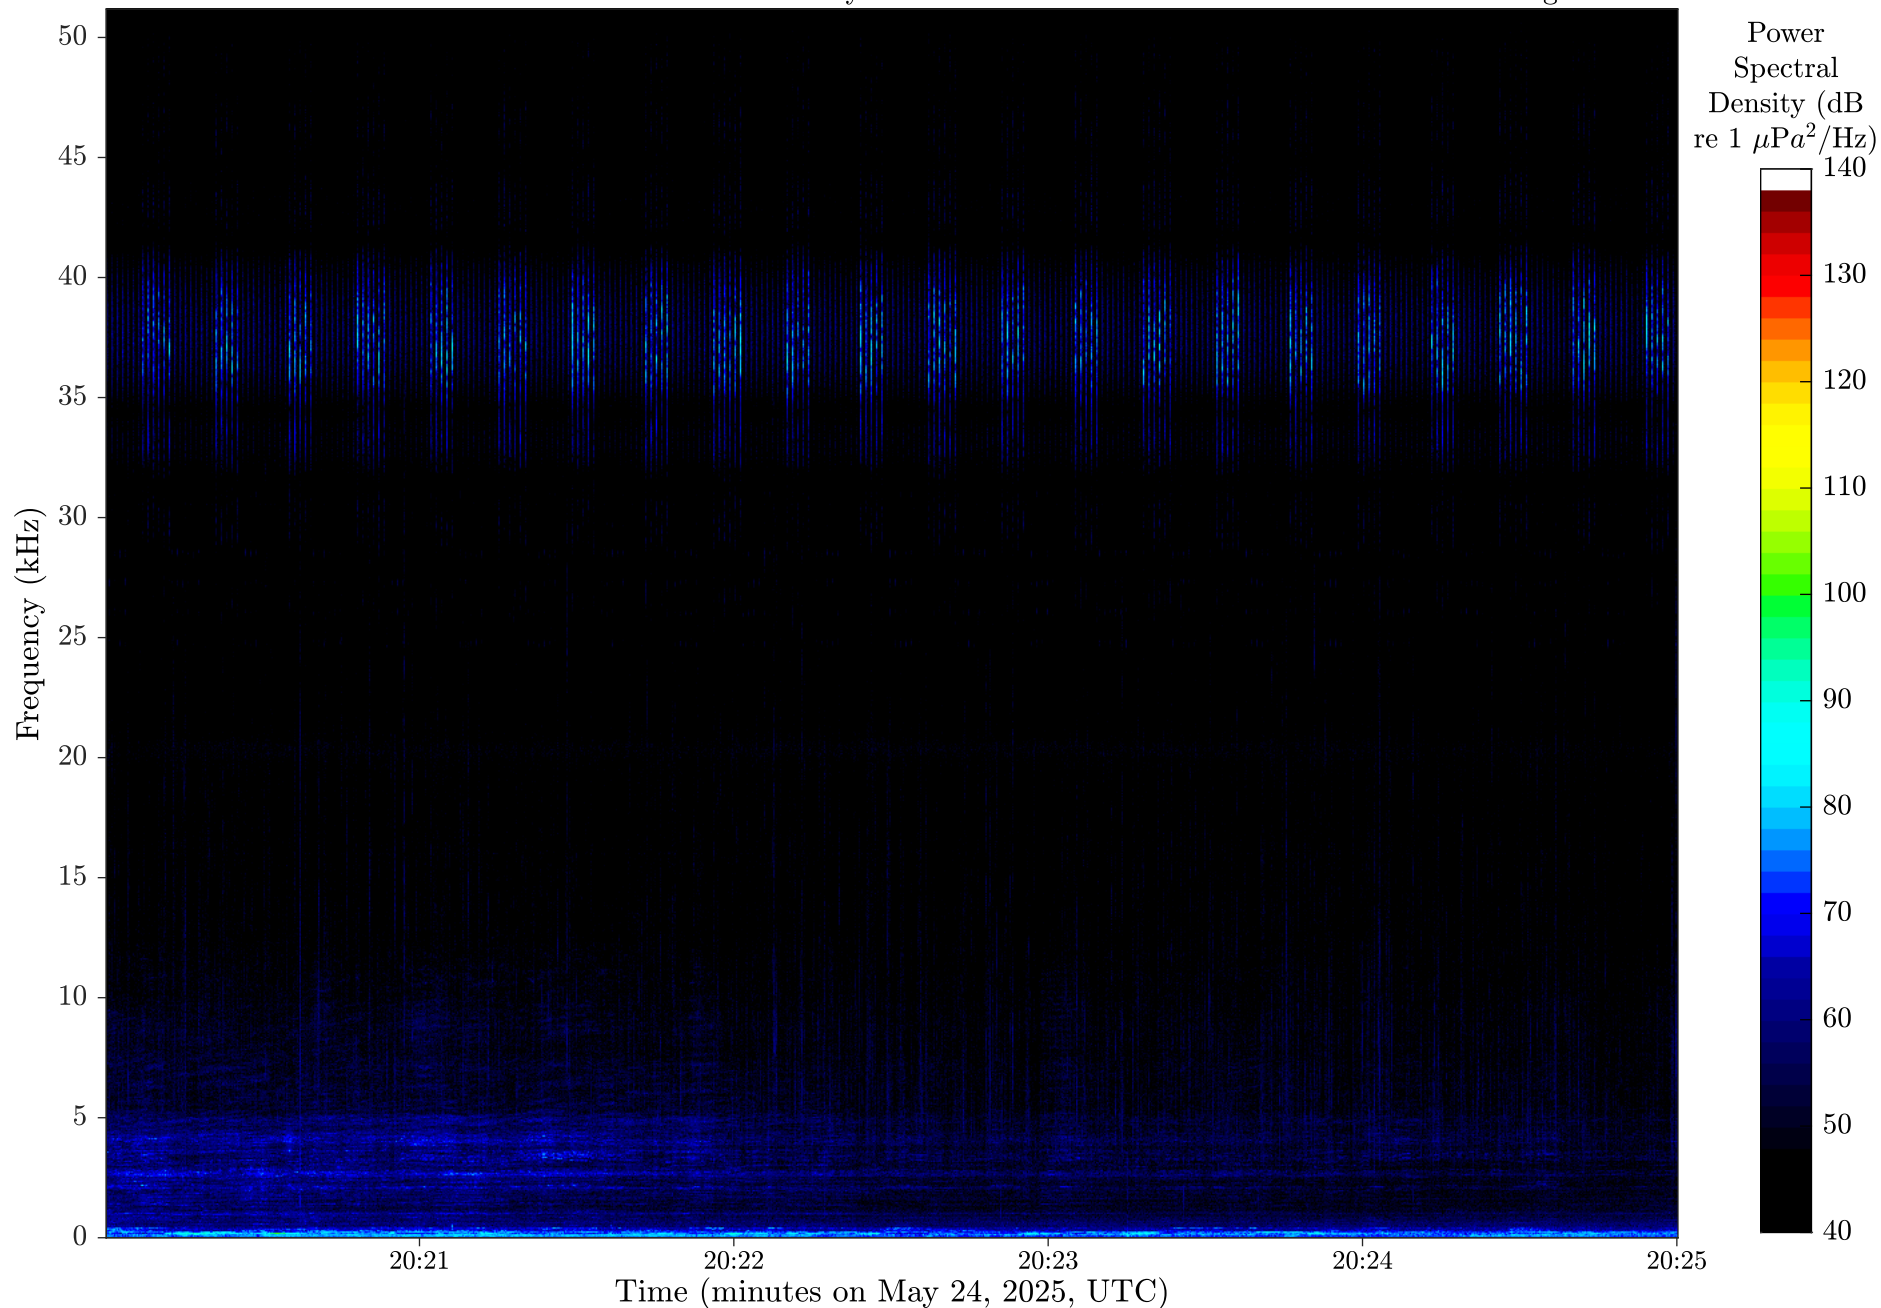


Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:50 UTC

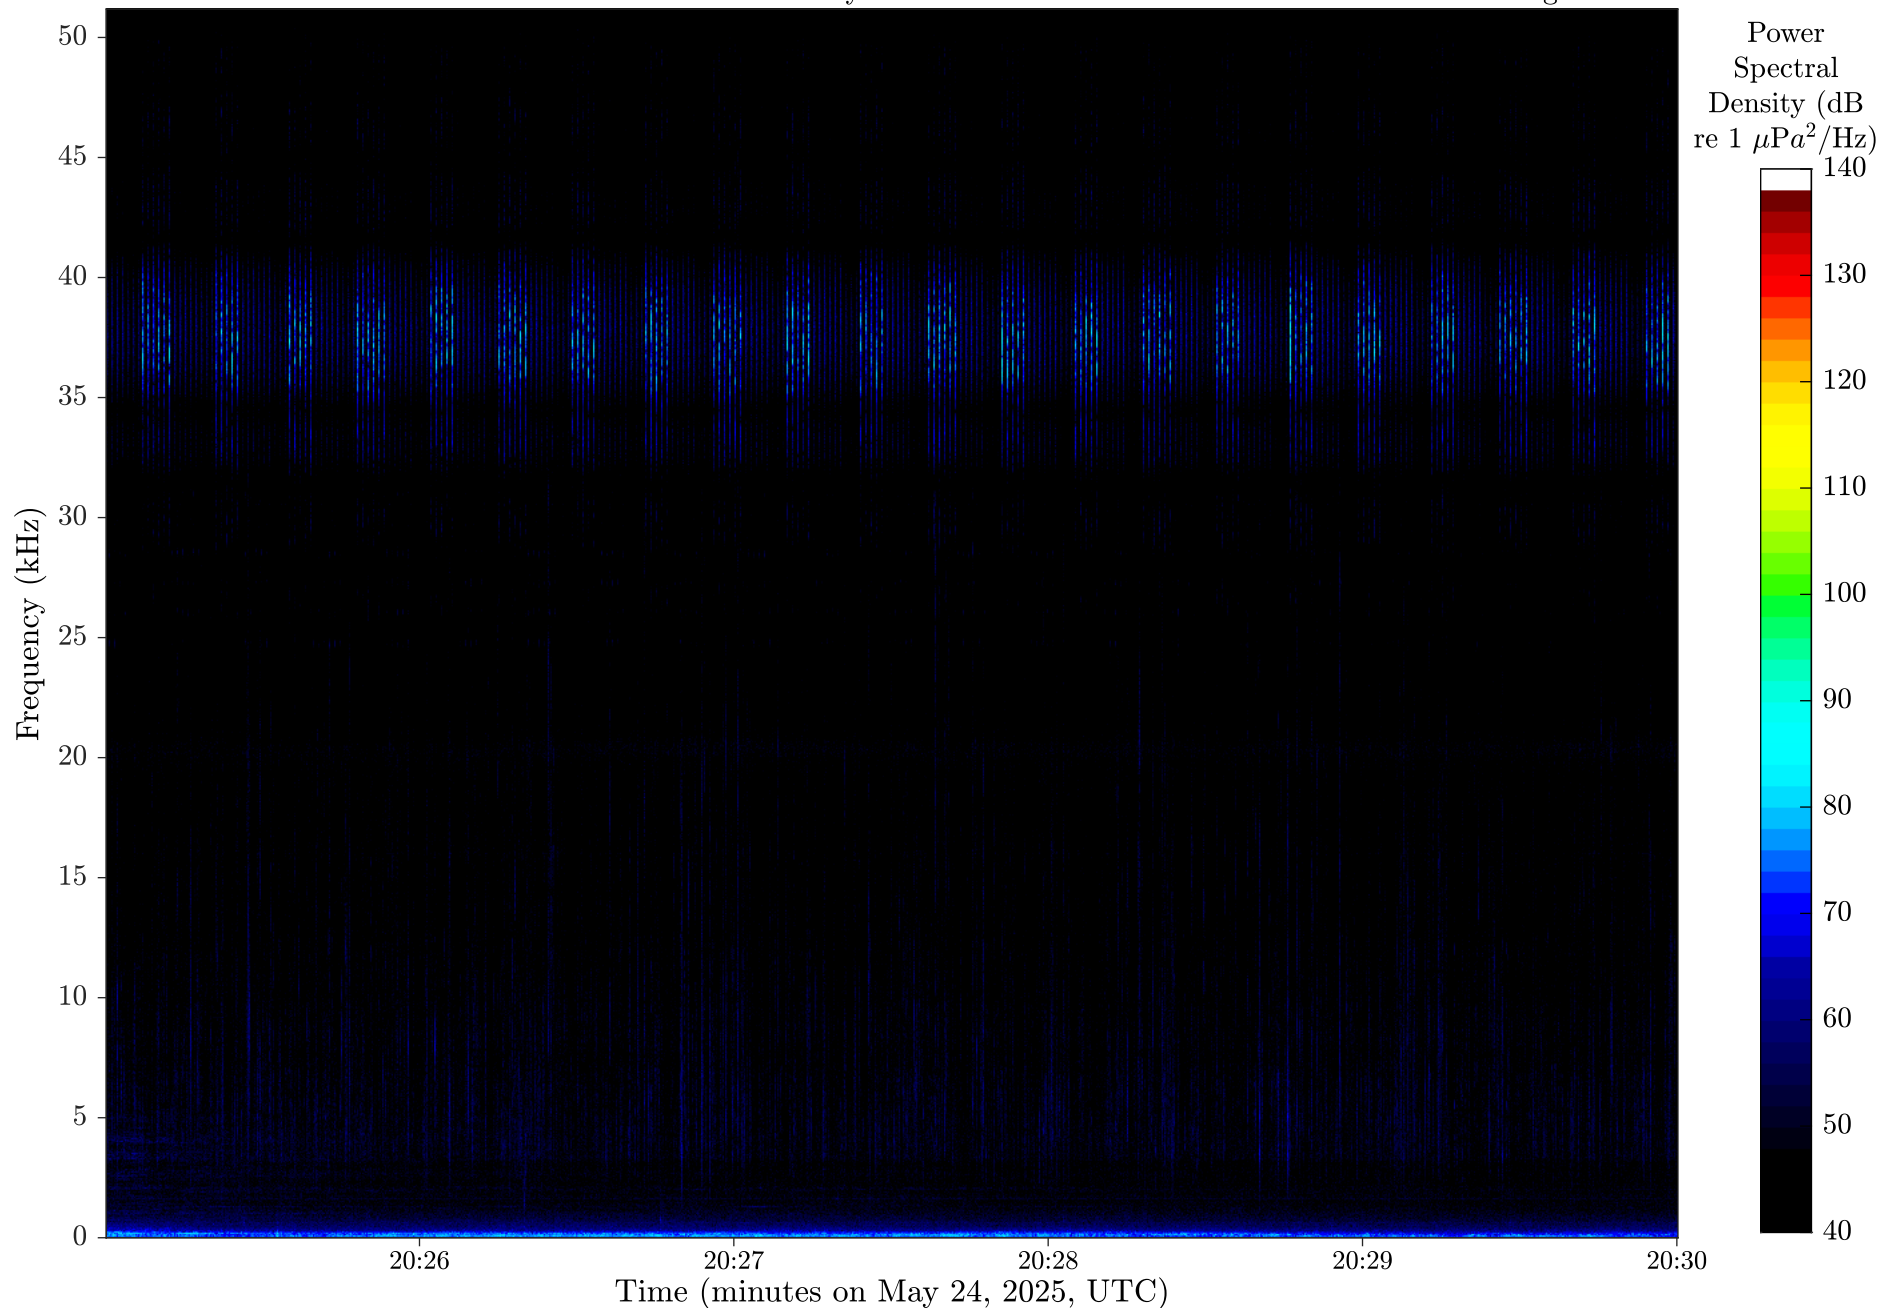


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:58 UTC

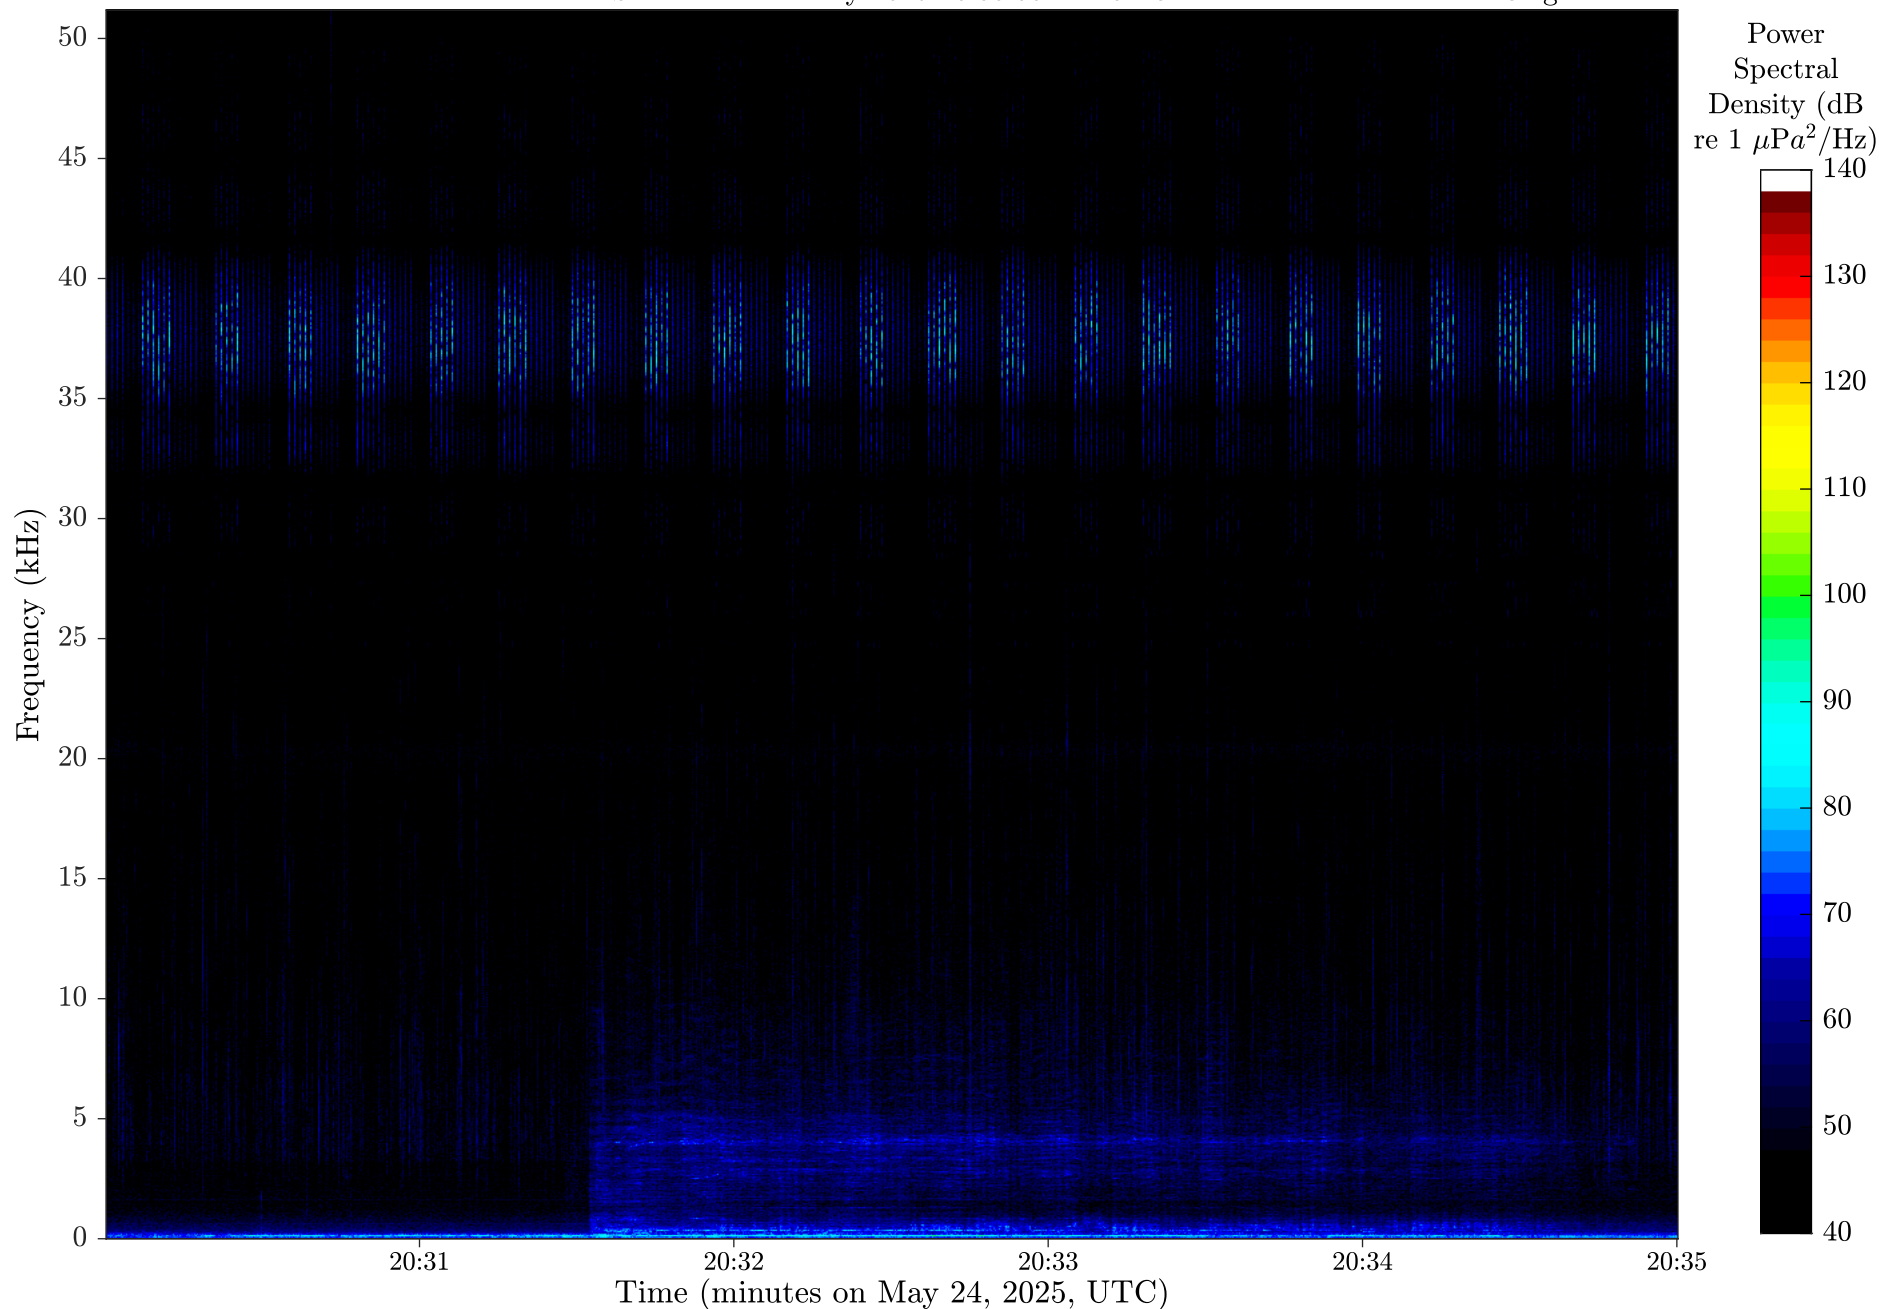


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:05 UTC

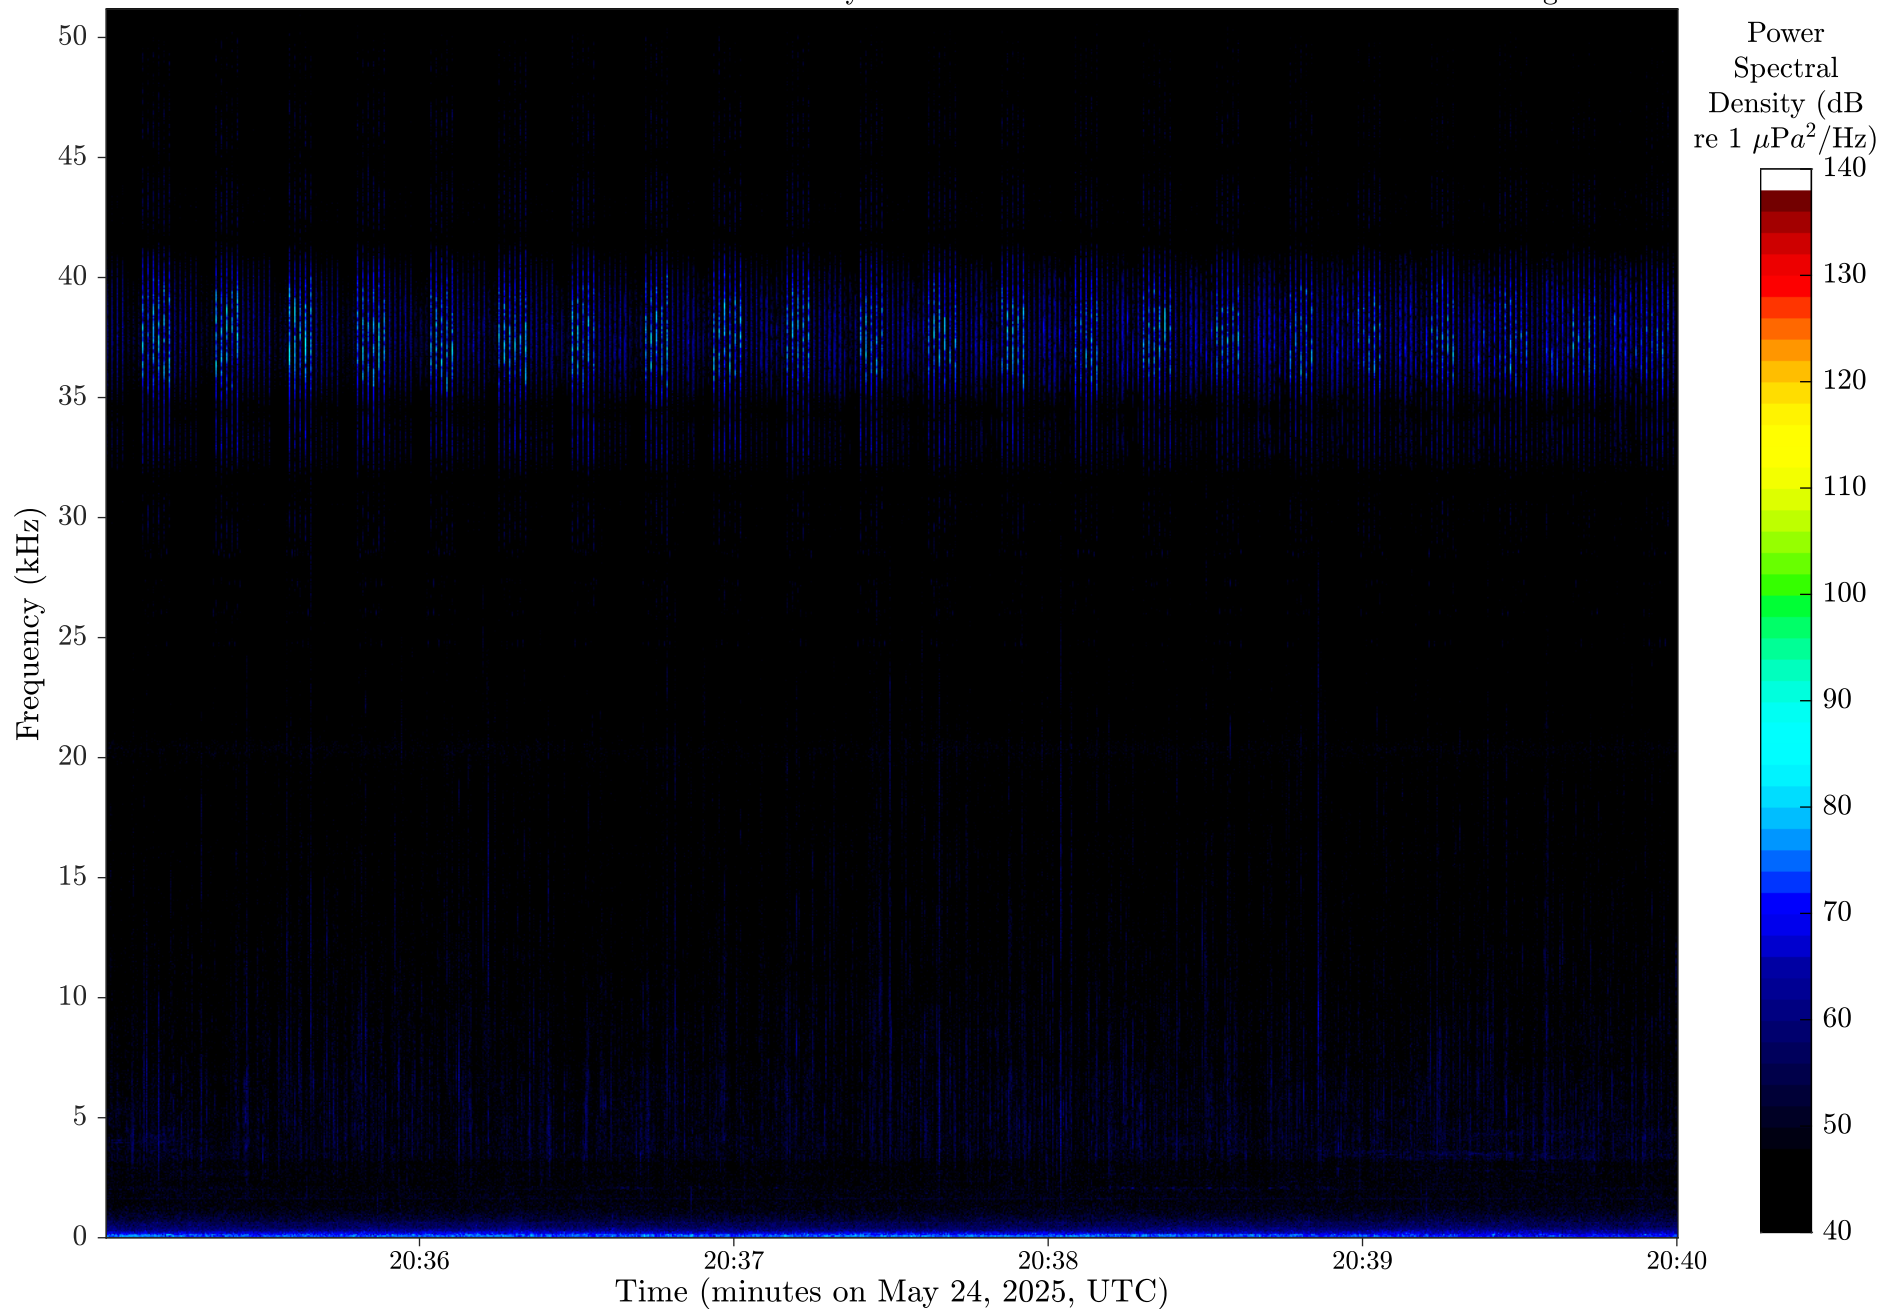


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:12 UTC

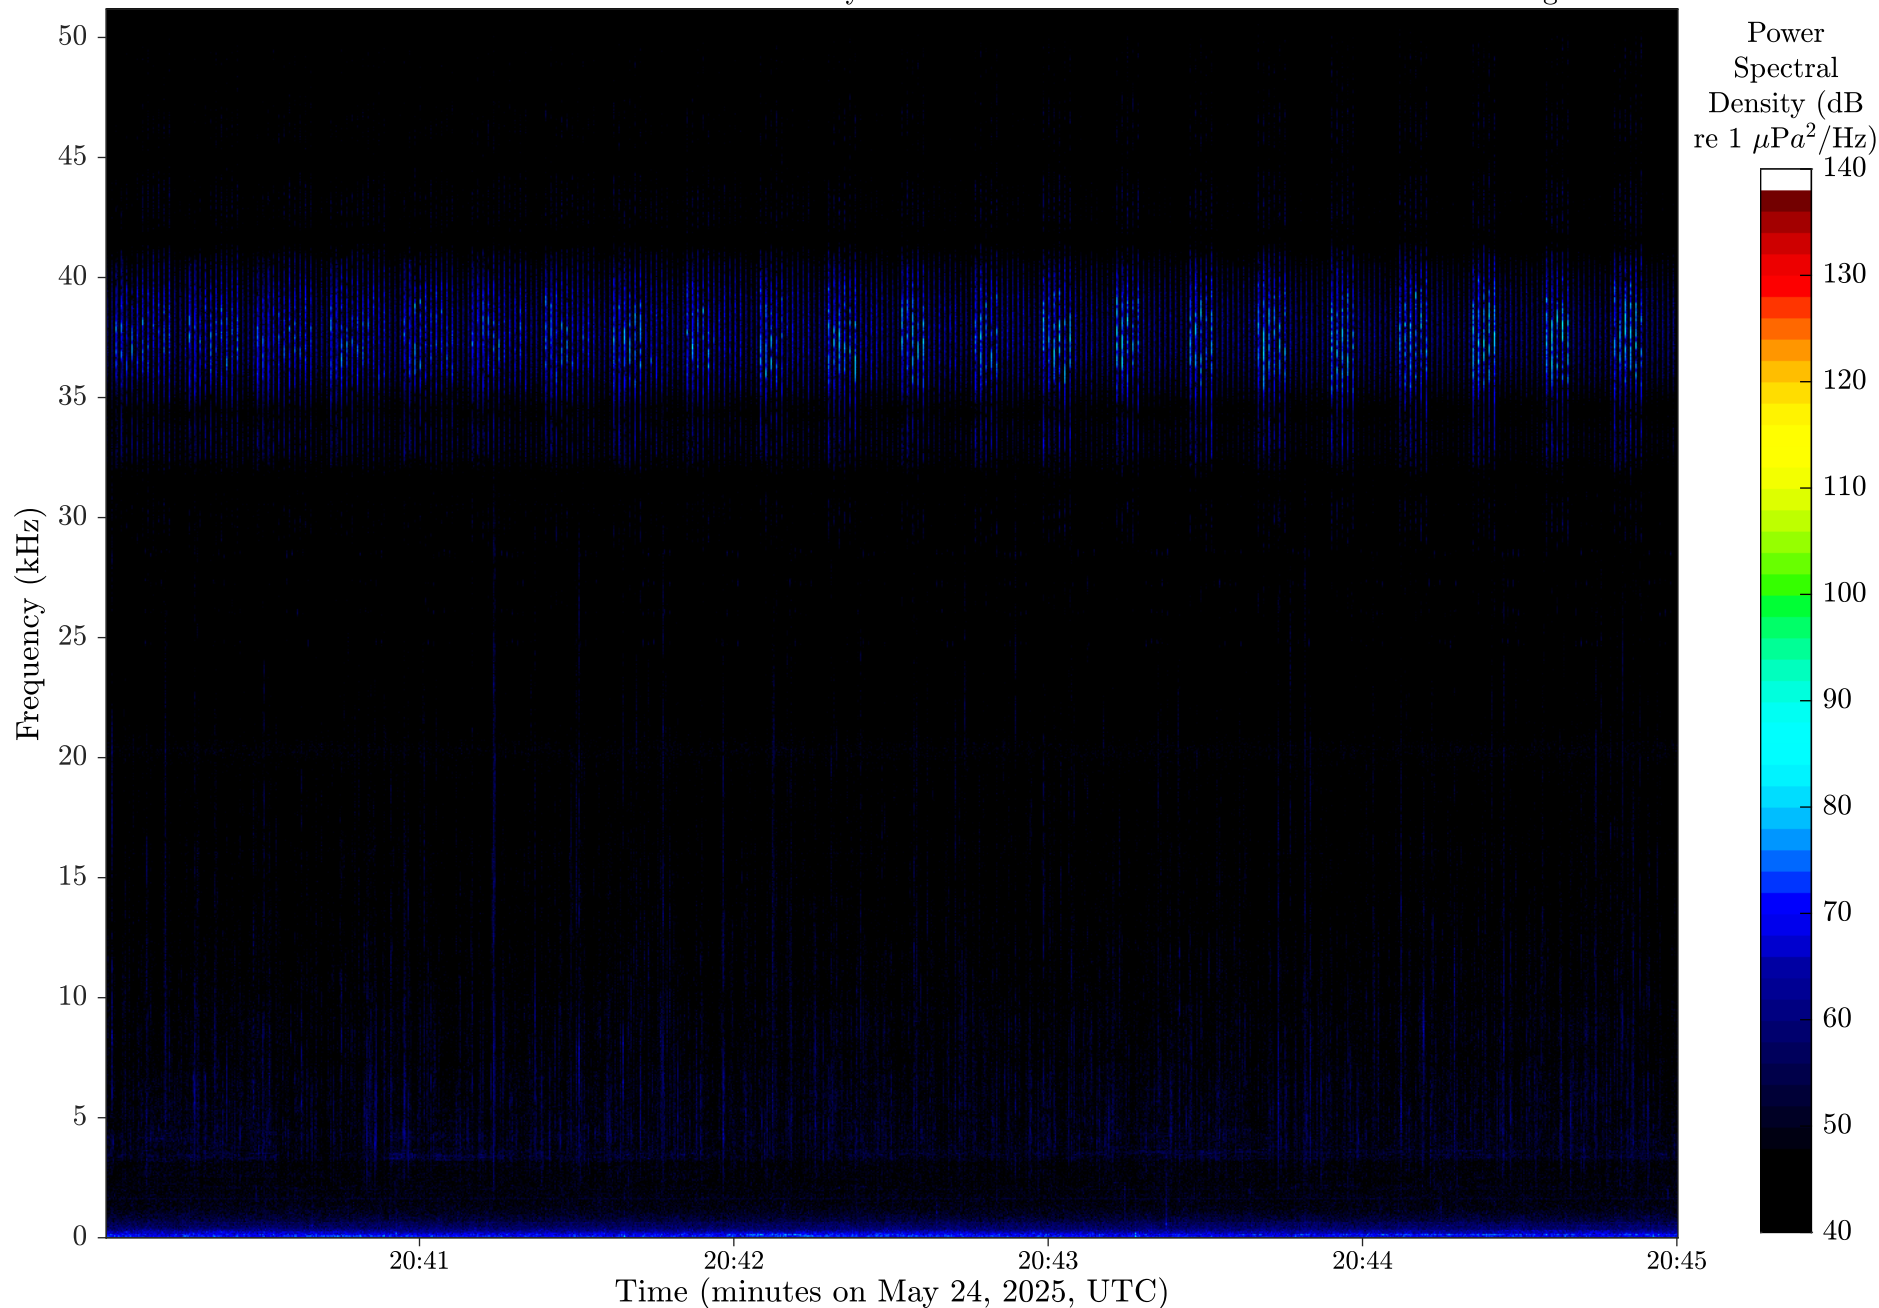


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:20 UTC

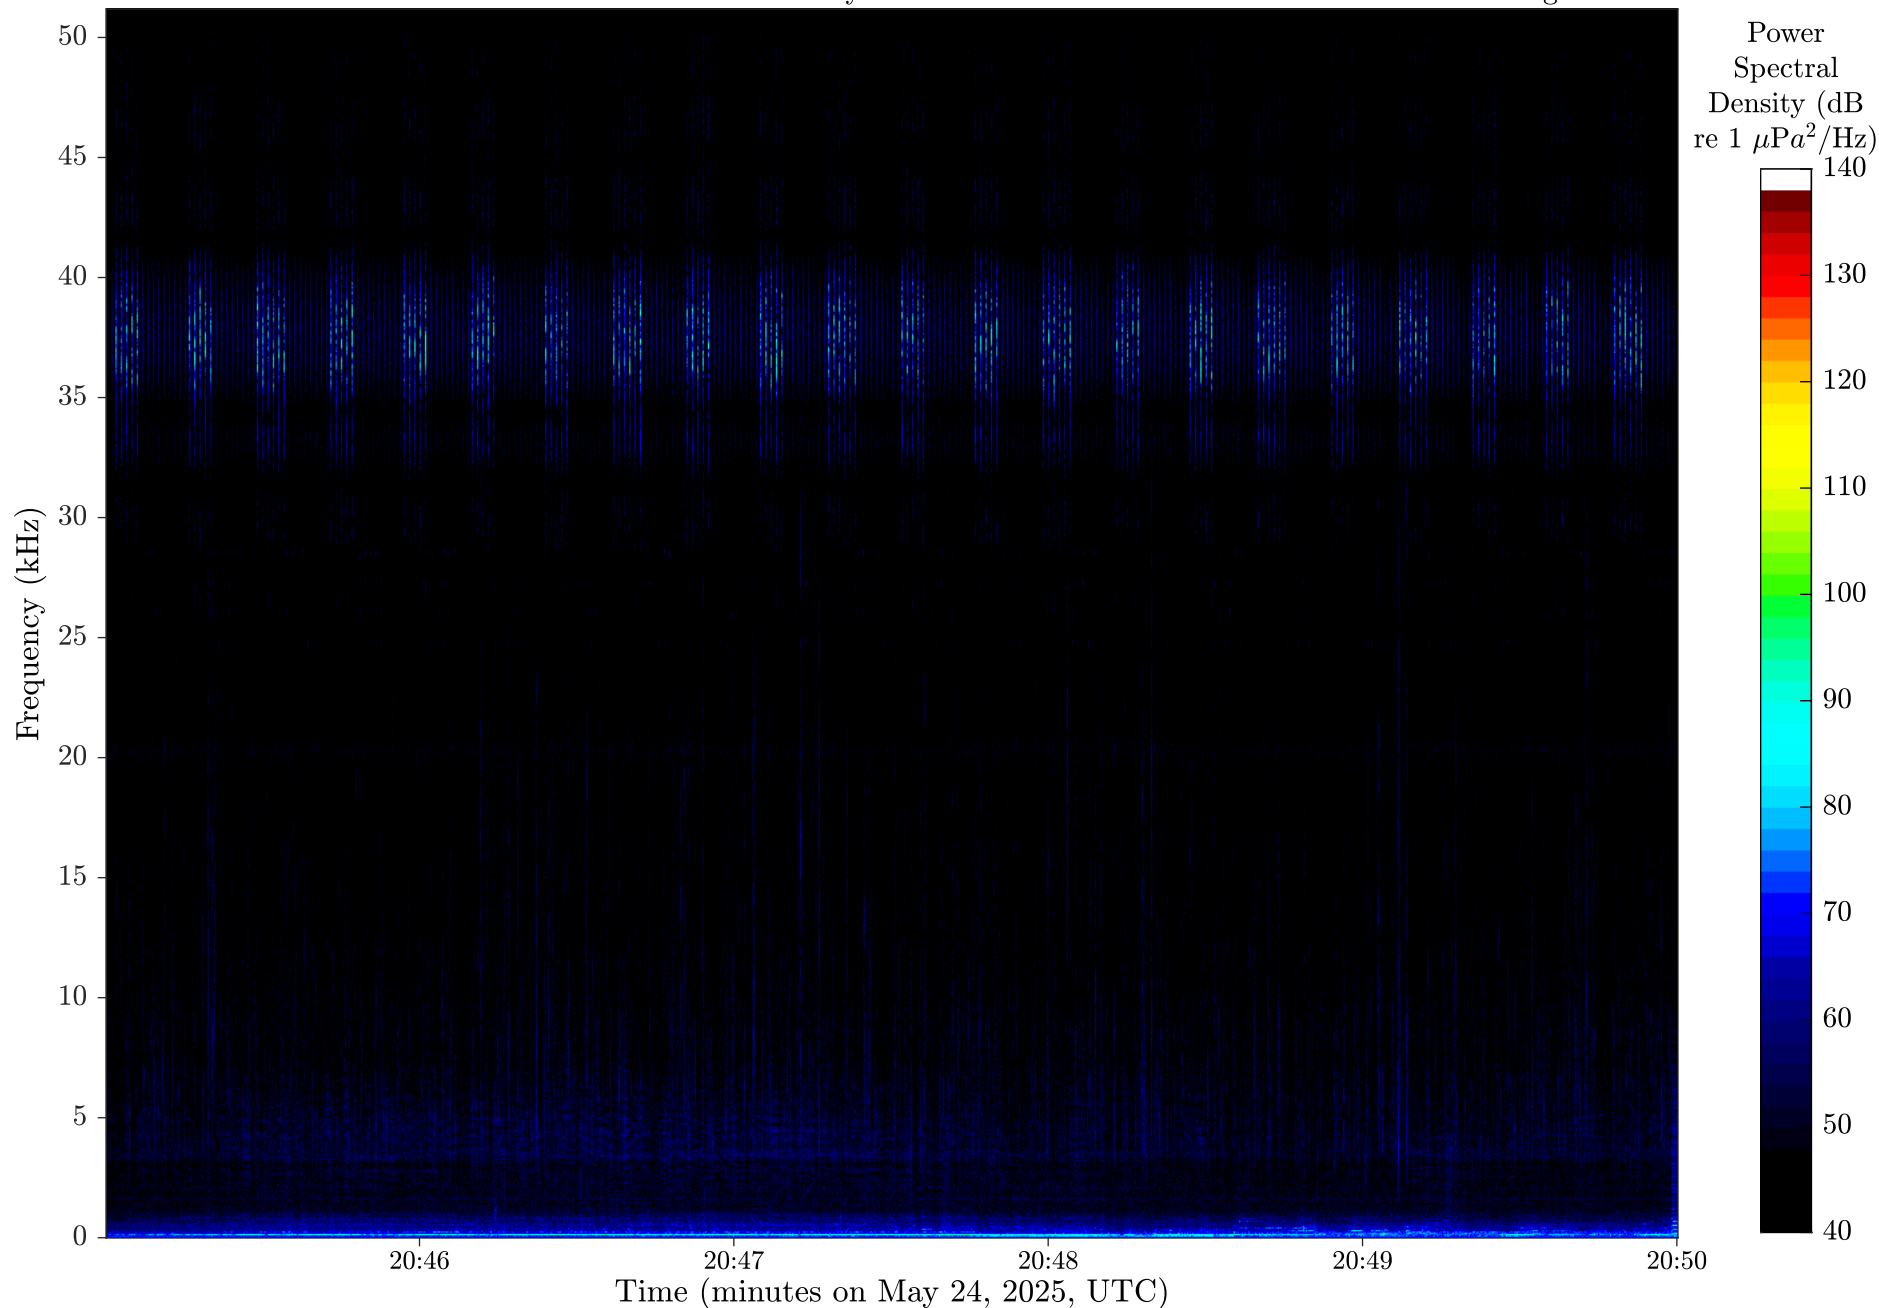


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:27 UTC

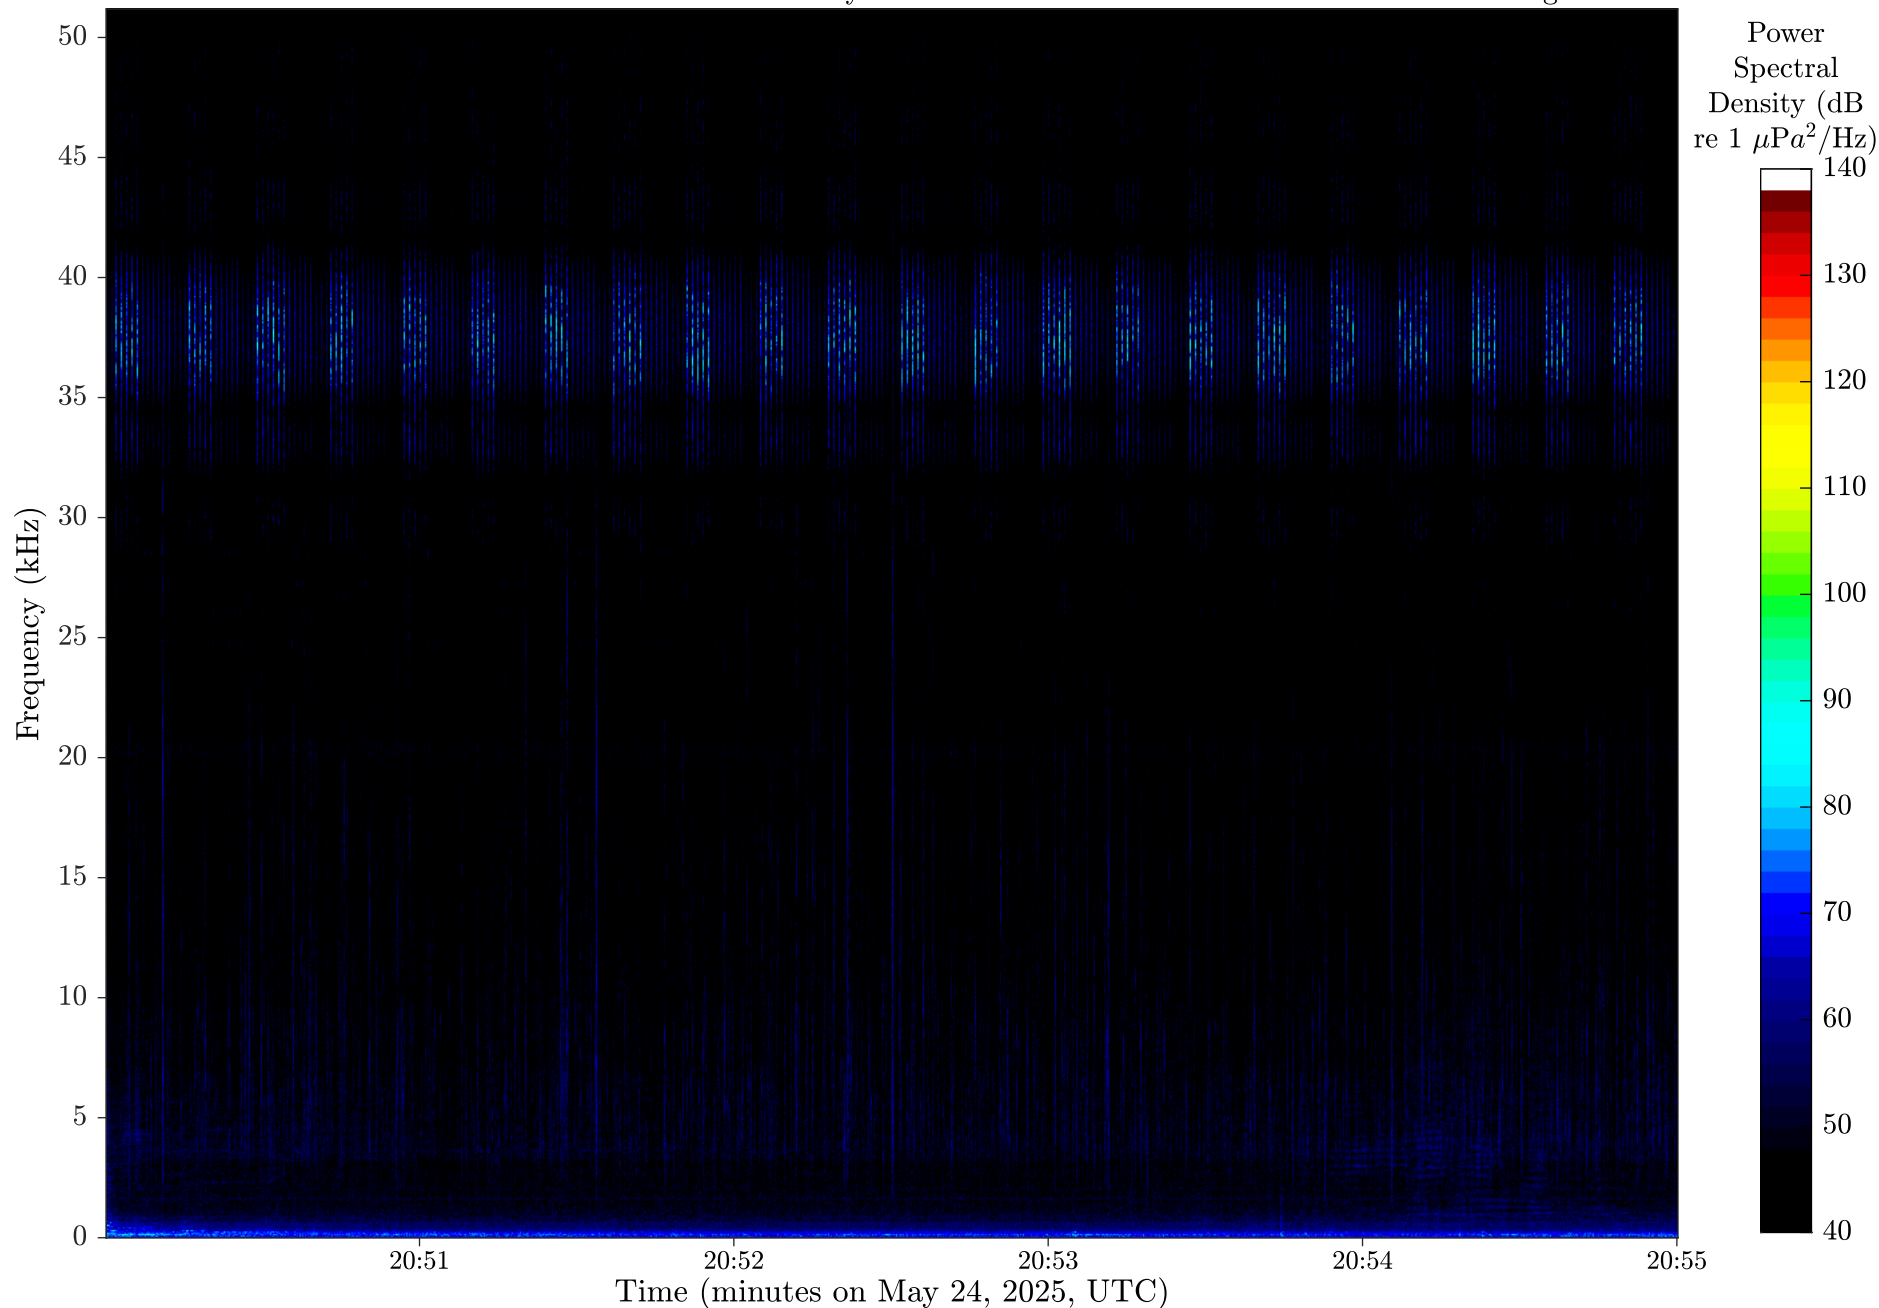


Comments: 33.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:34 UTC

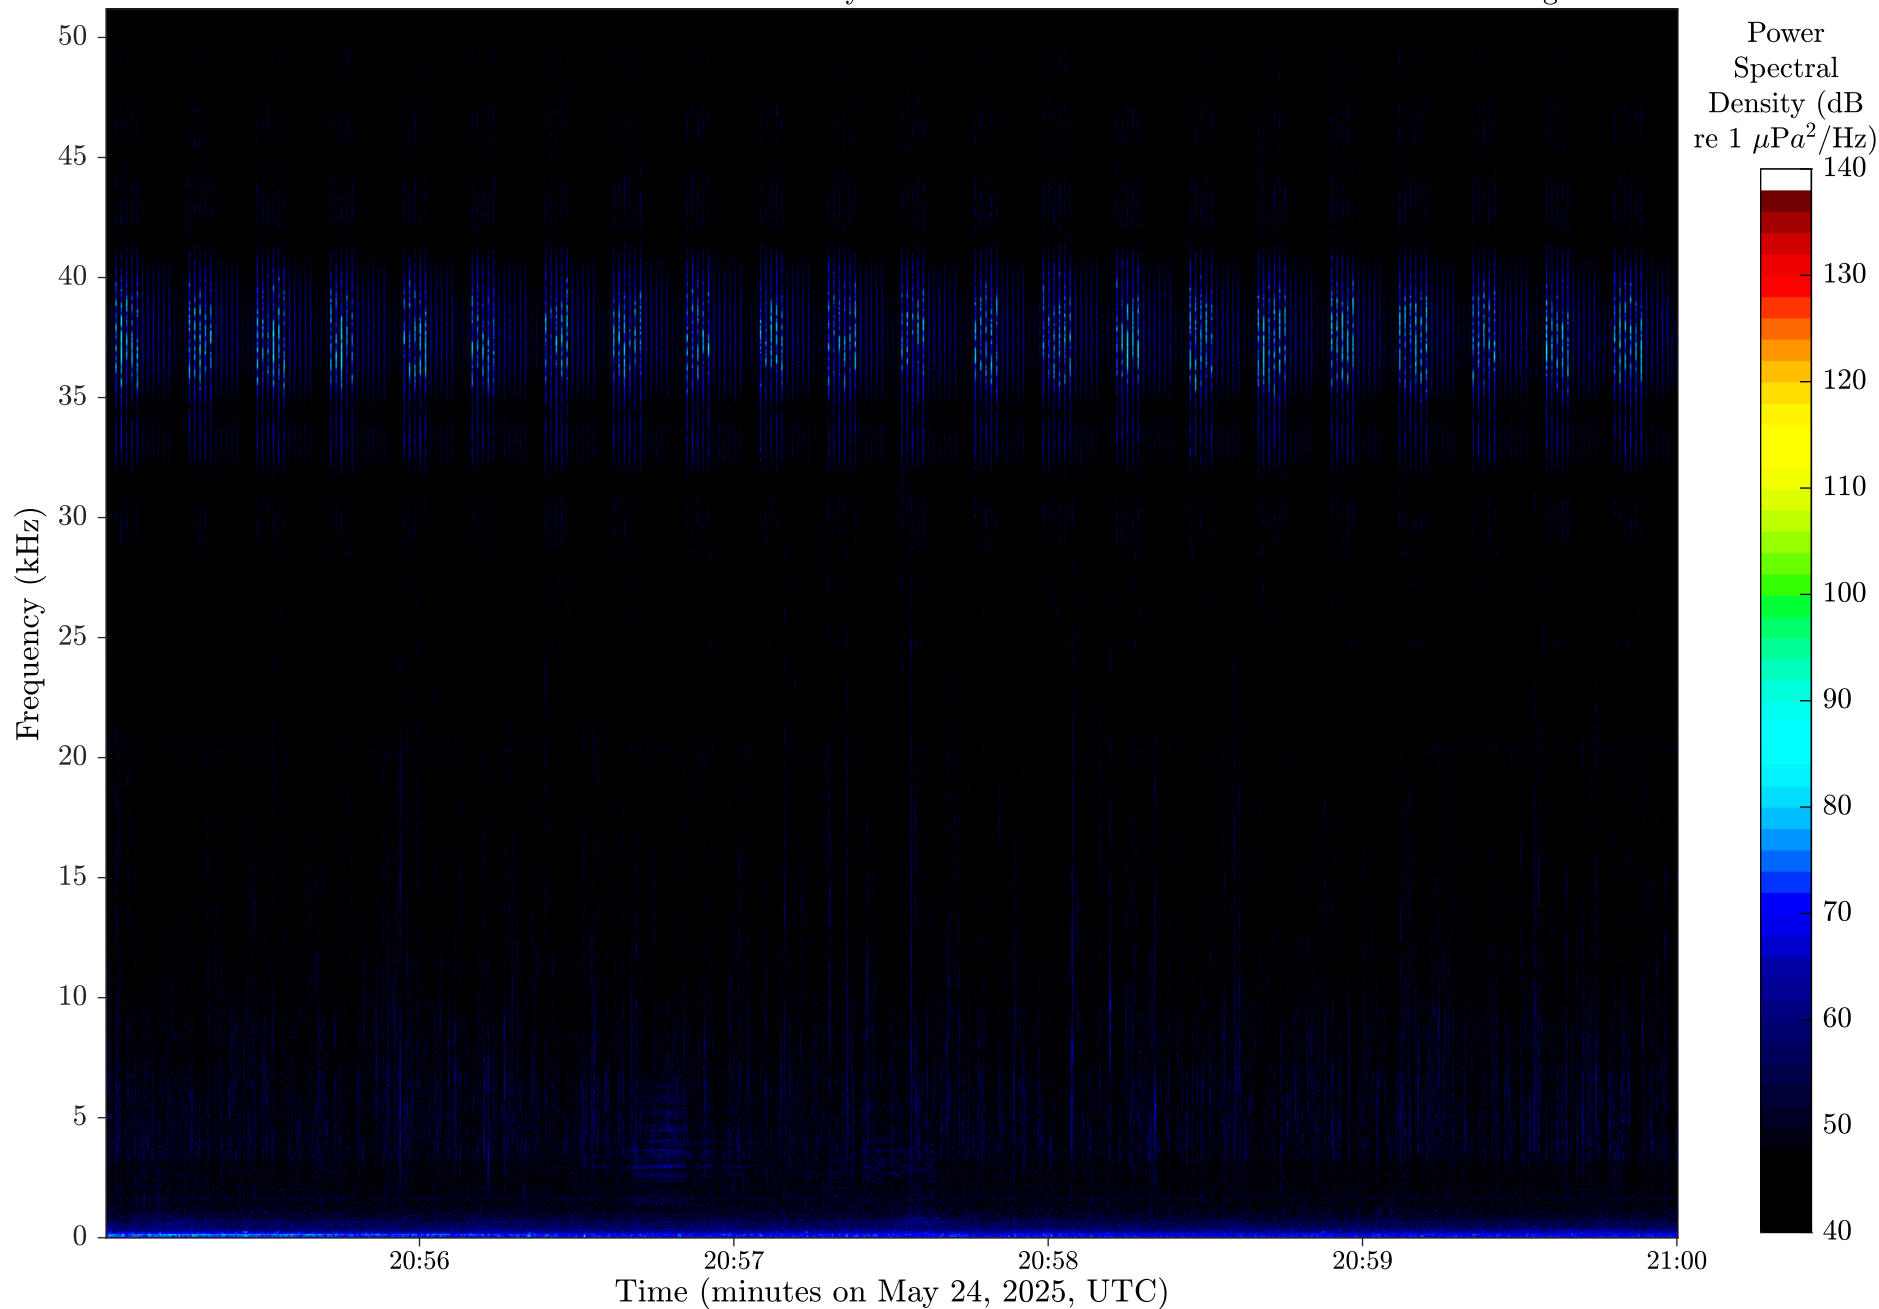


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:41 UTC

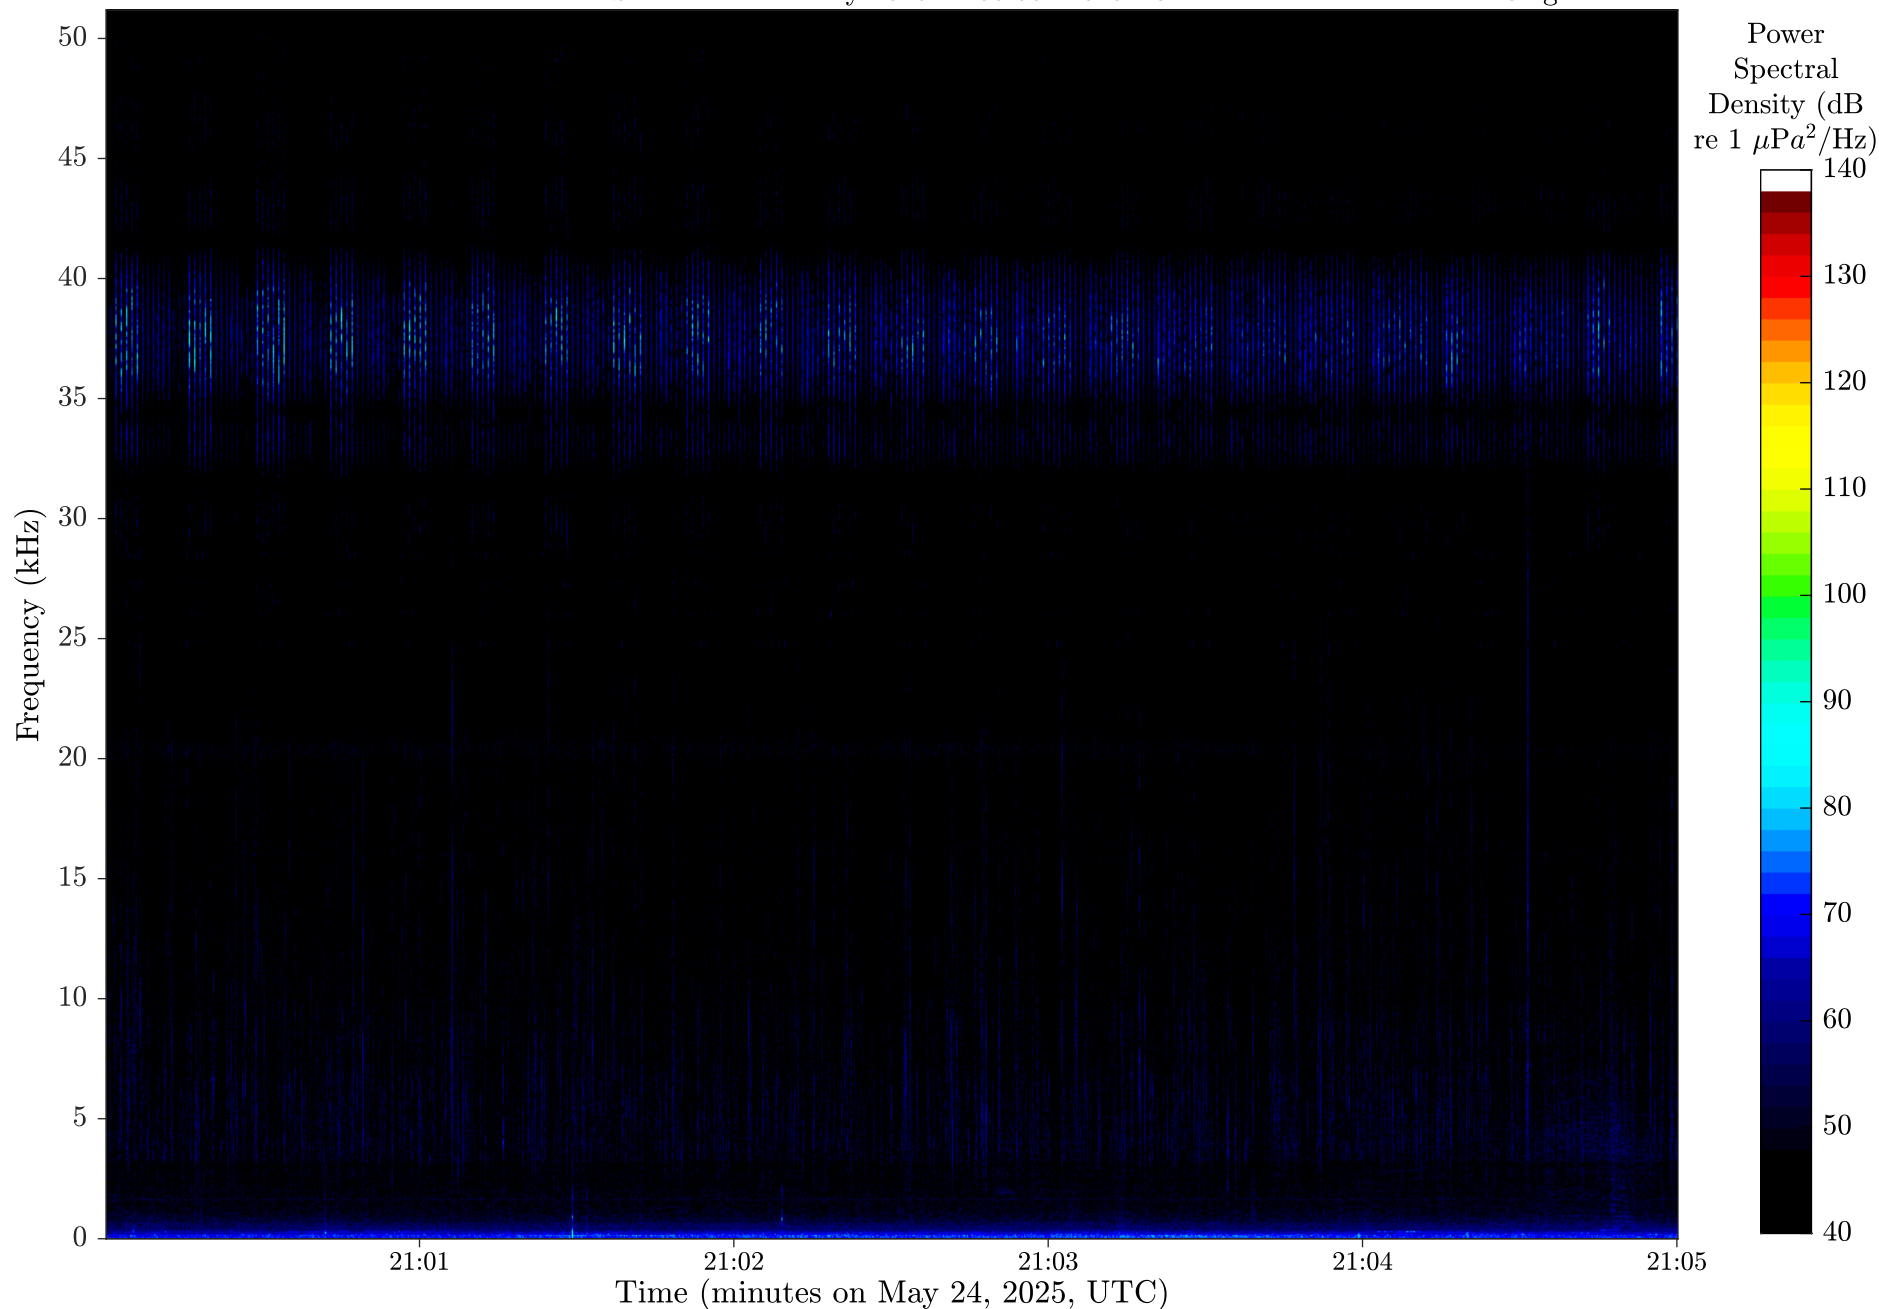


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:49 UTC

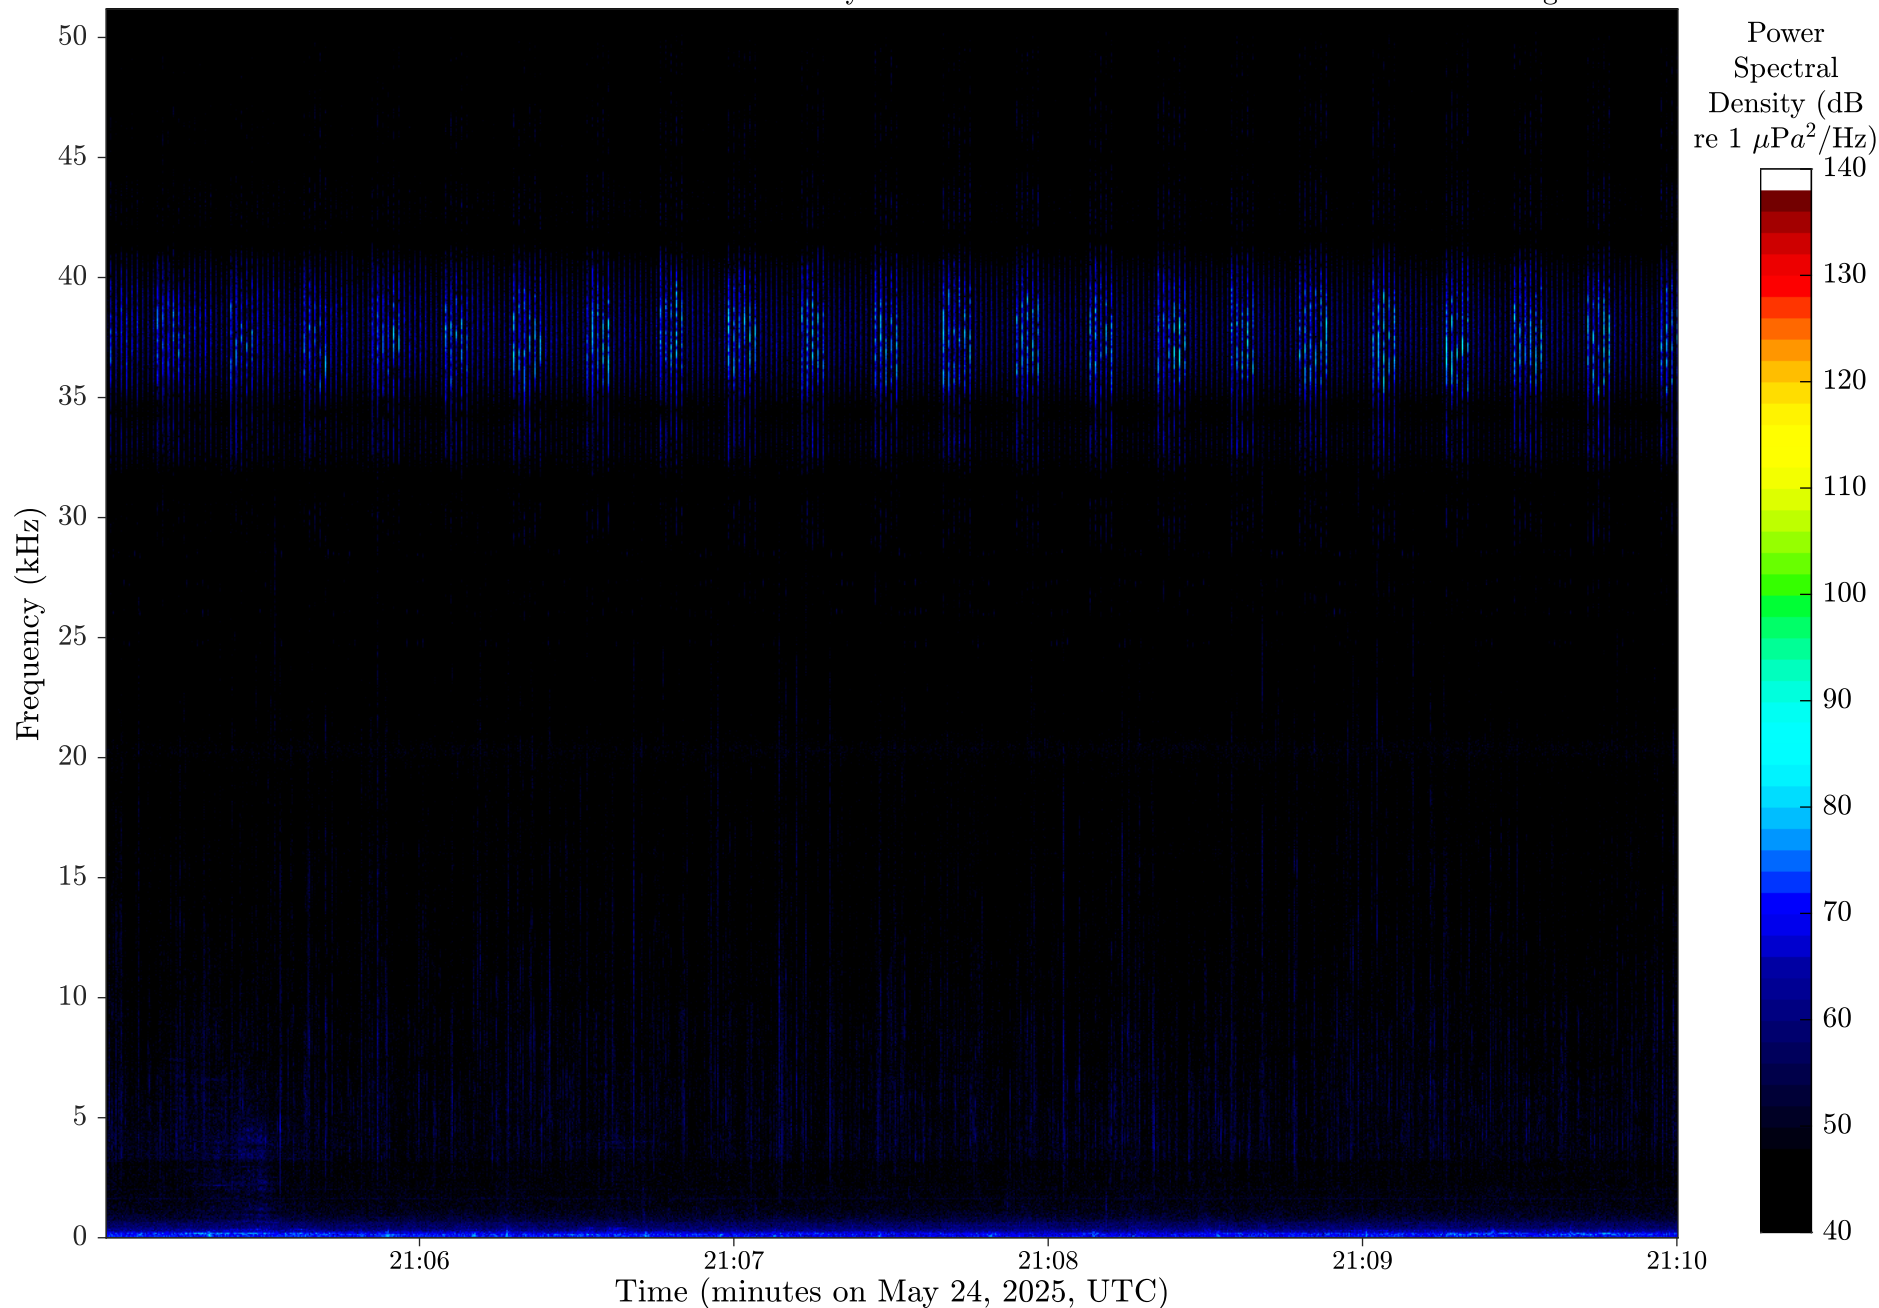


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:56 UTC

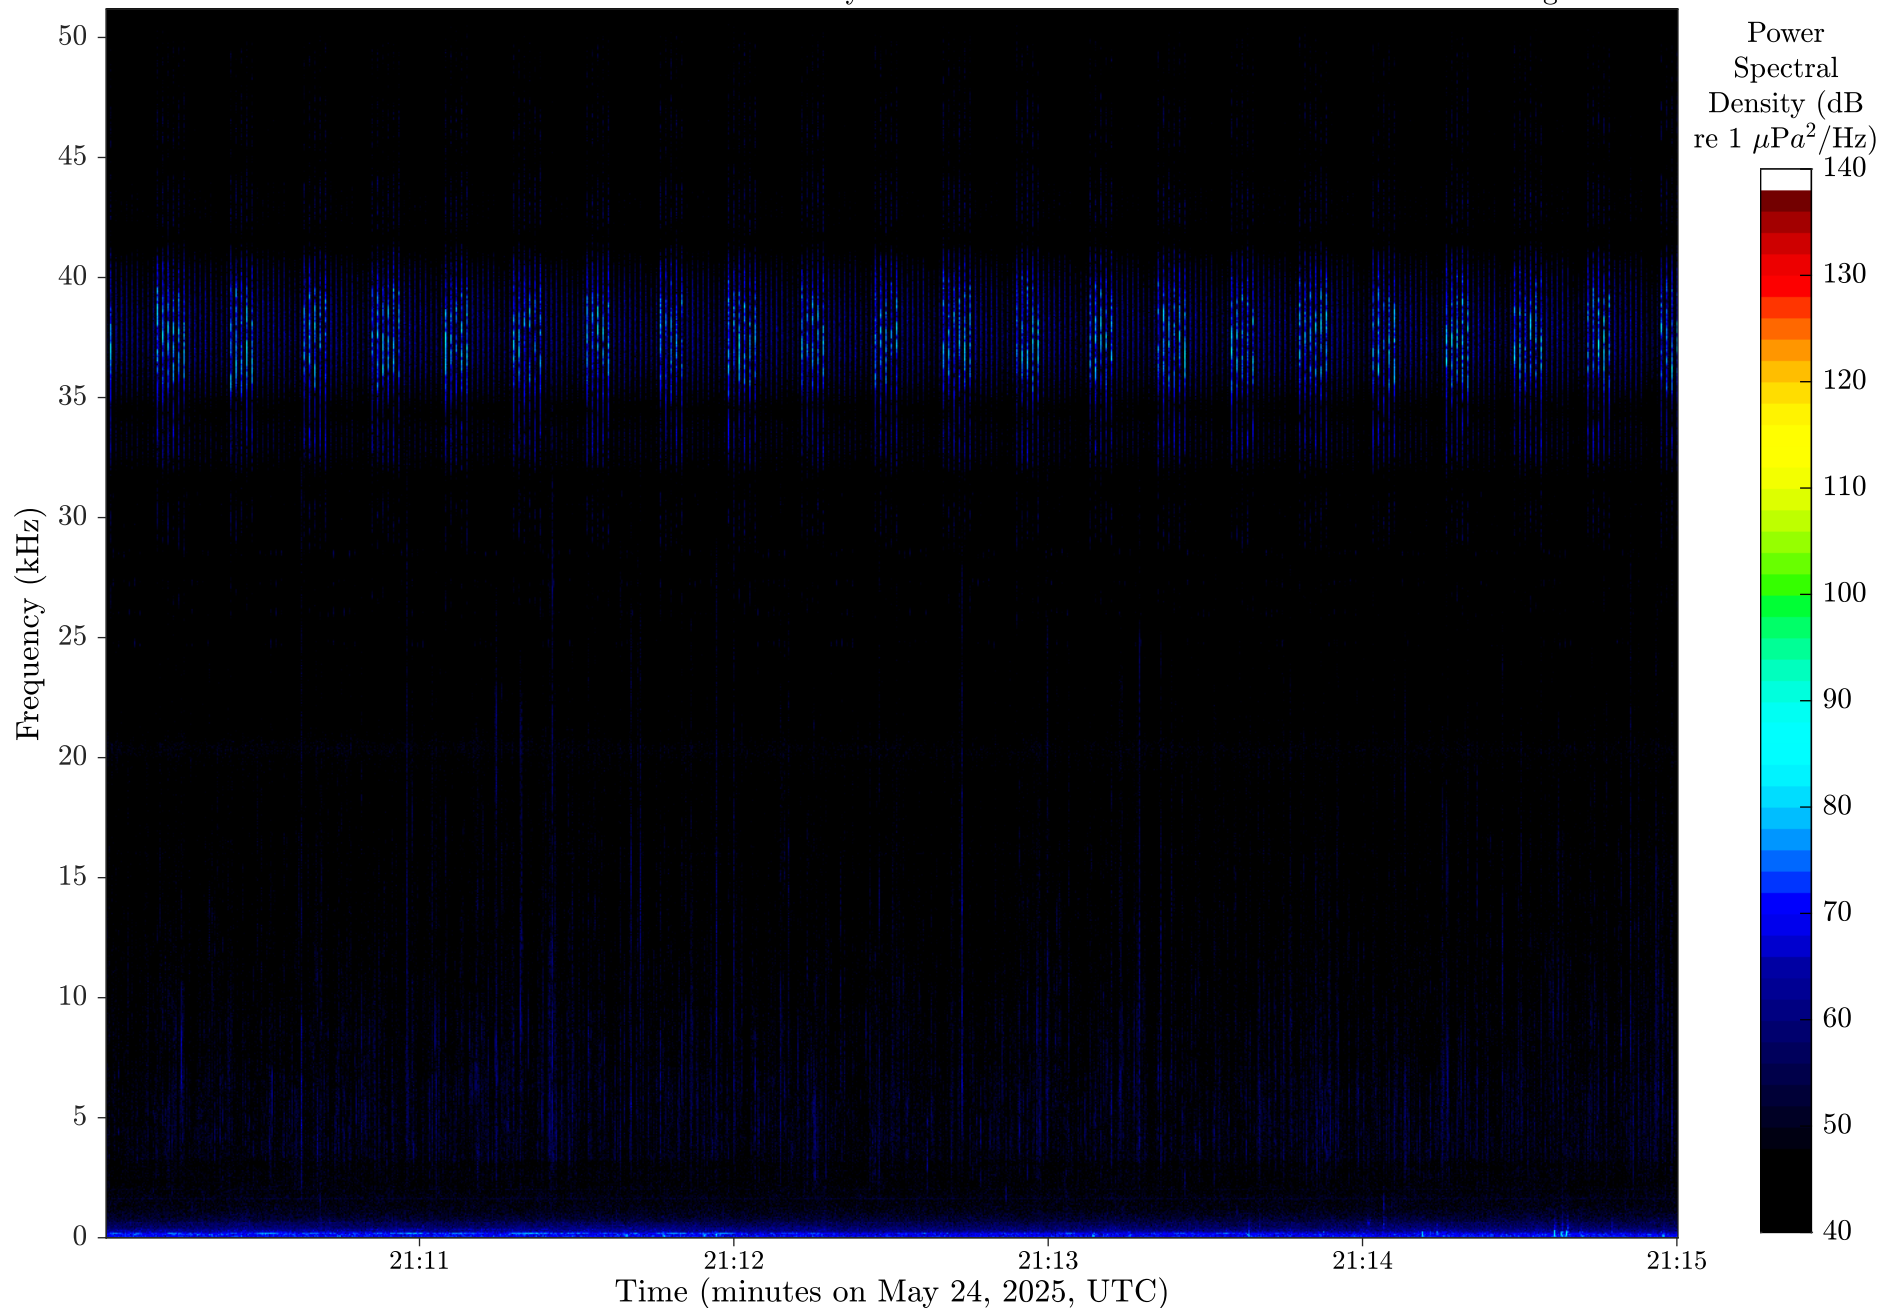


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:43:03 UTC

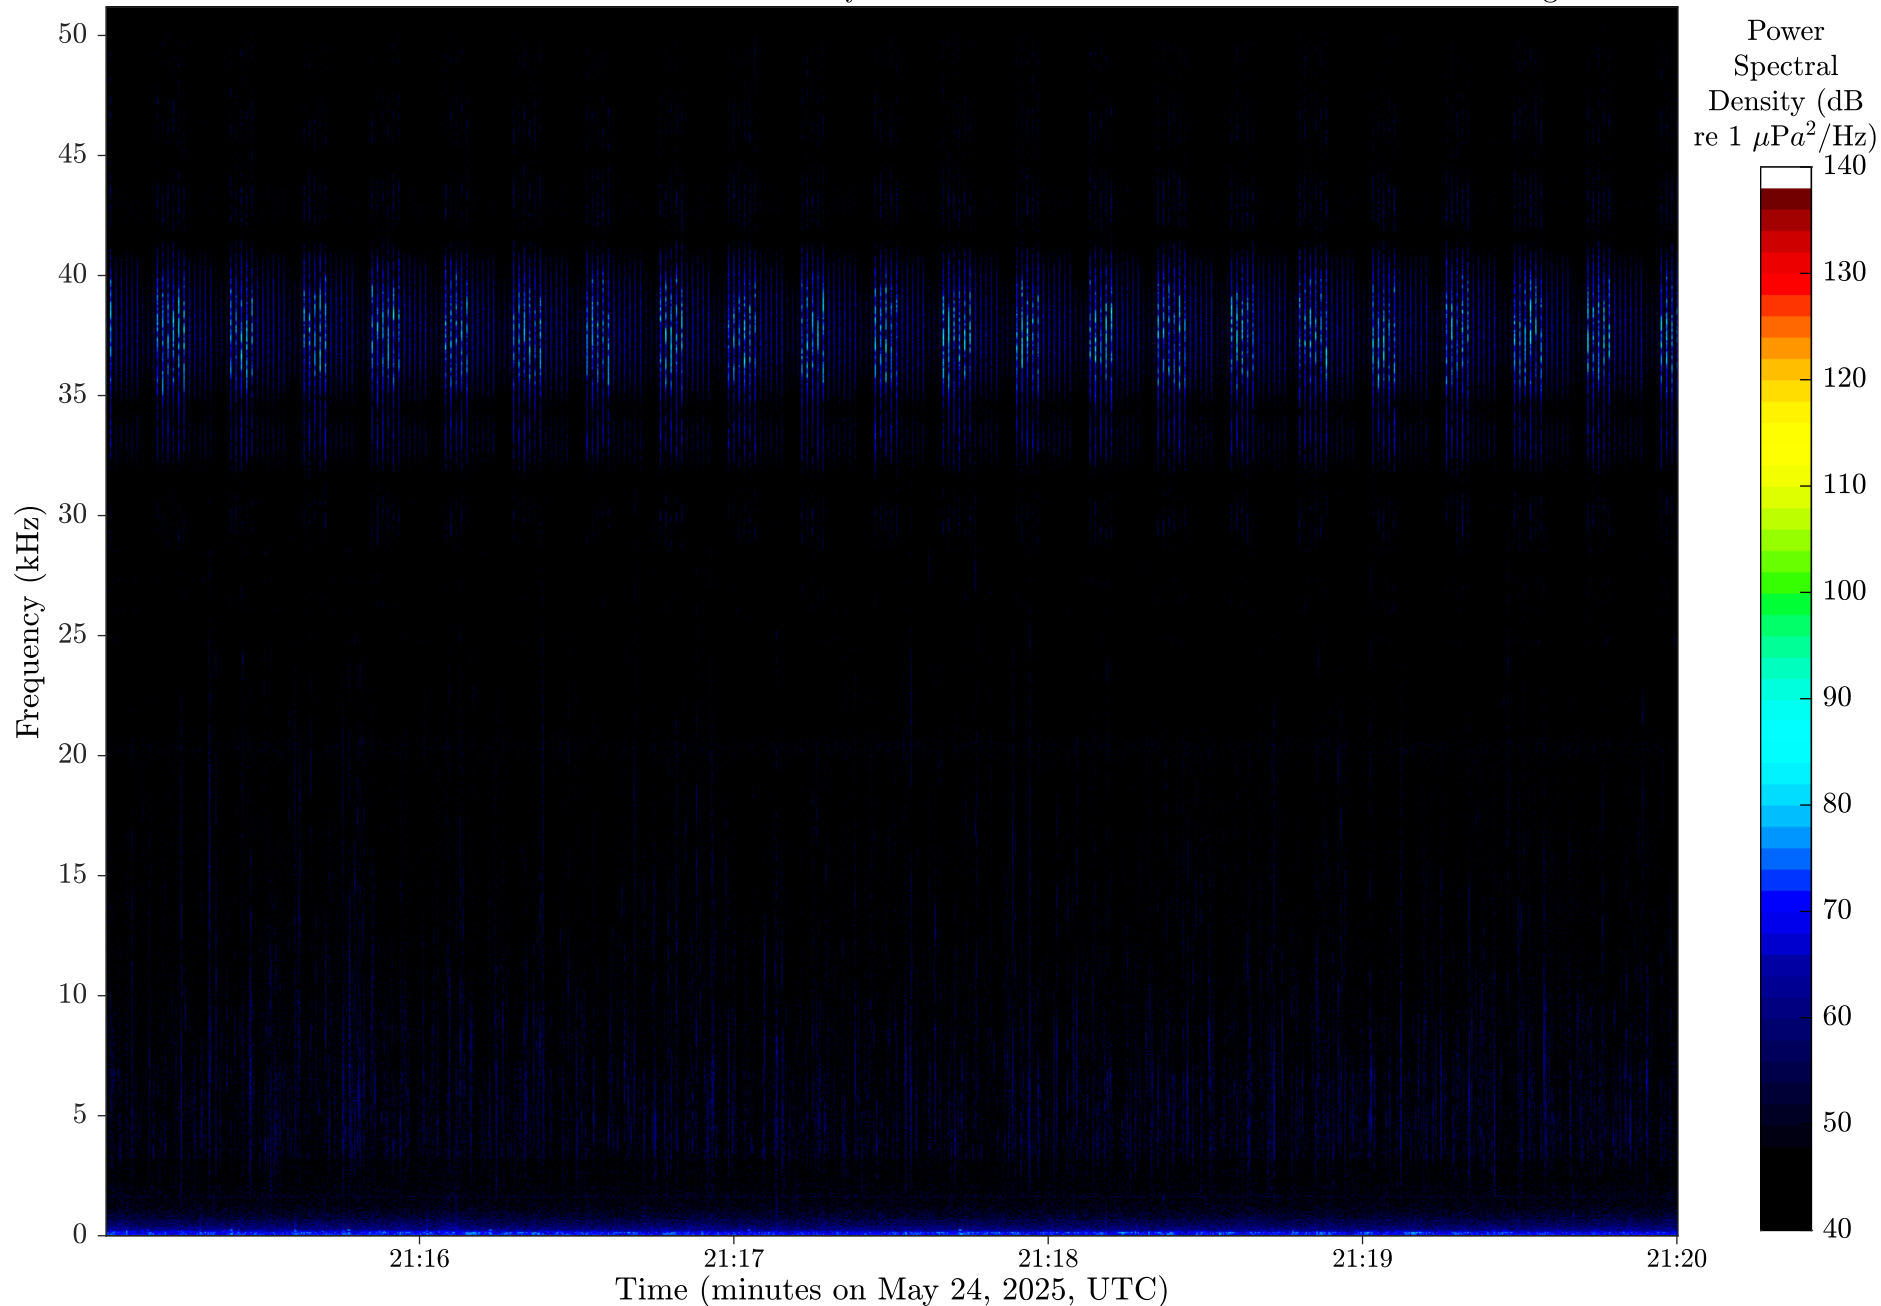


Comments: 34.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:43:10 UTC

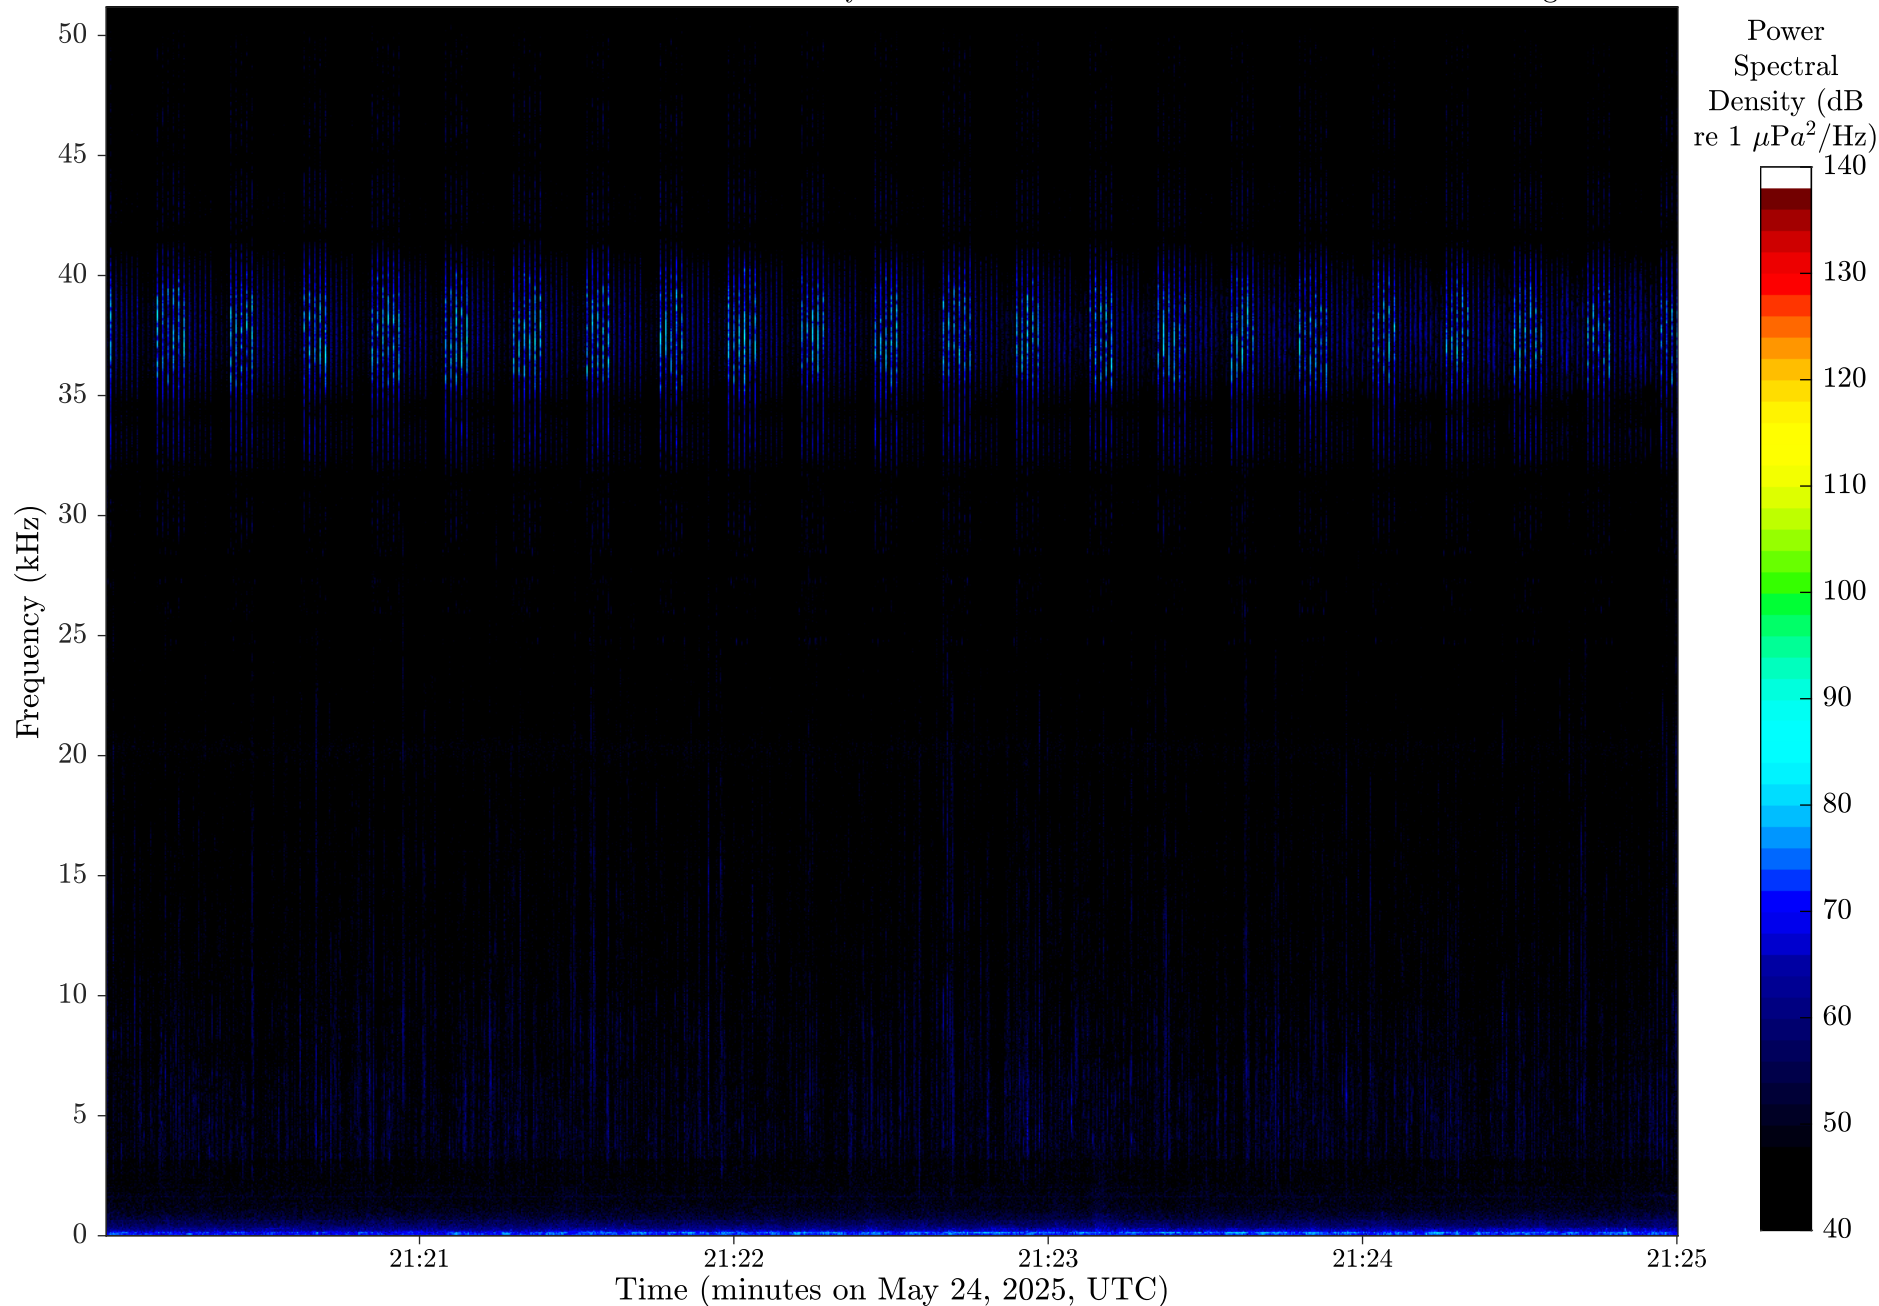

Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:43:17 UTC

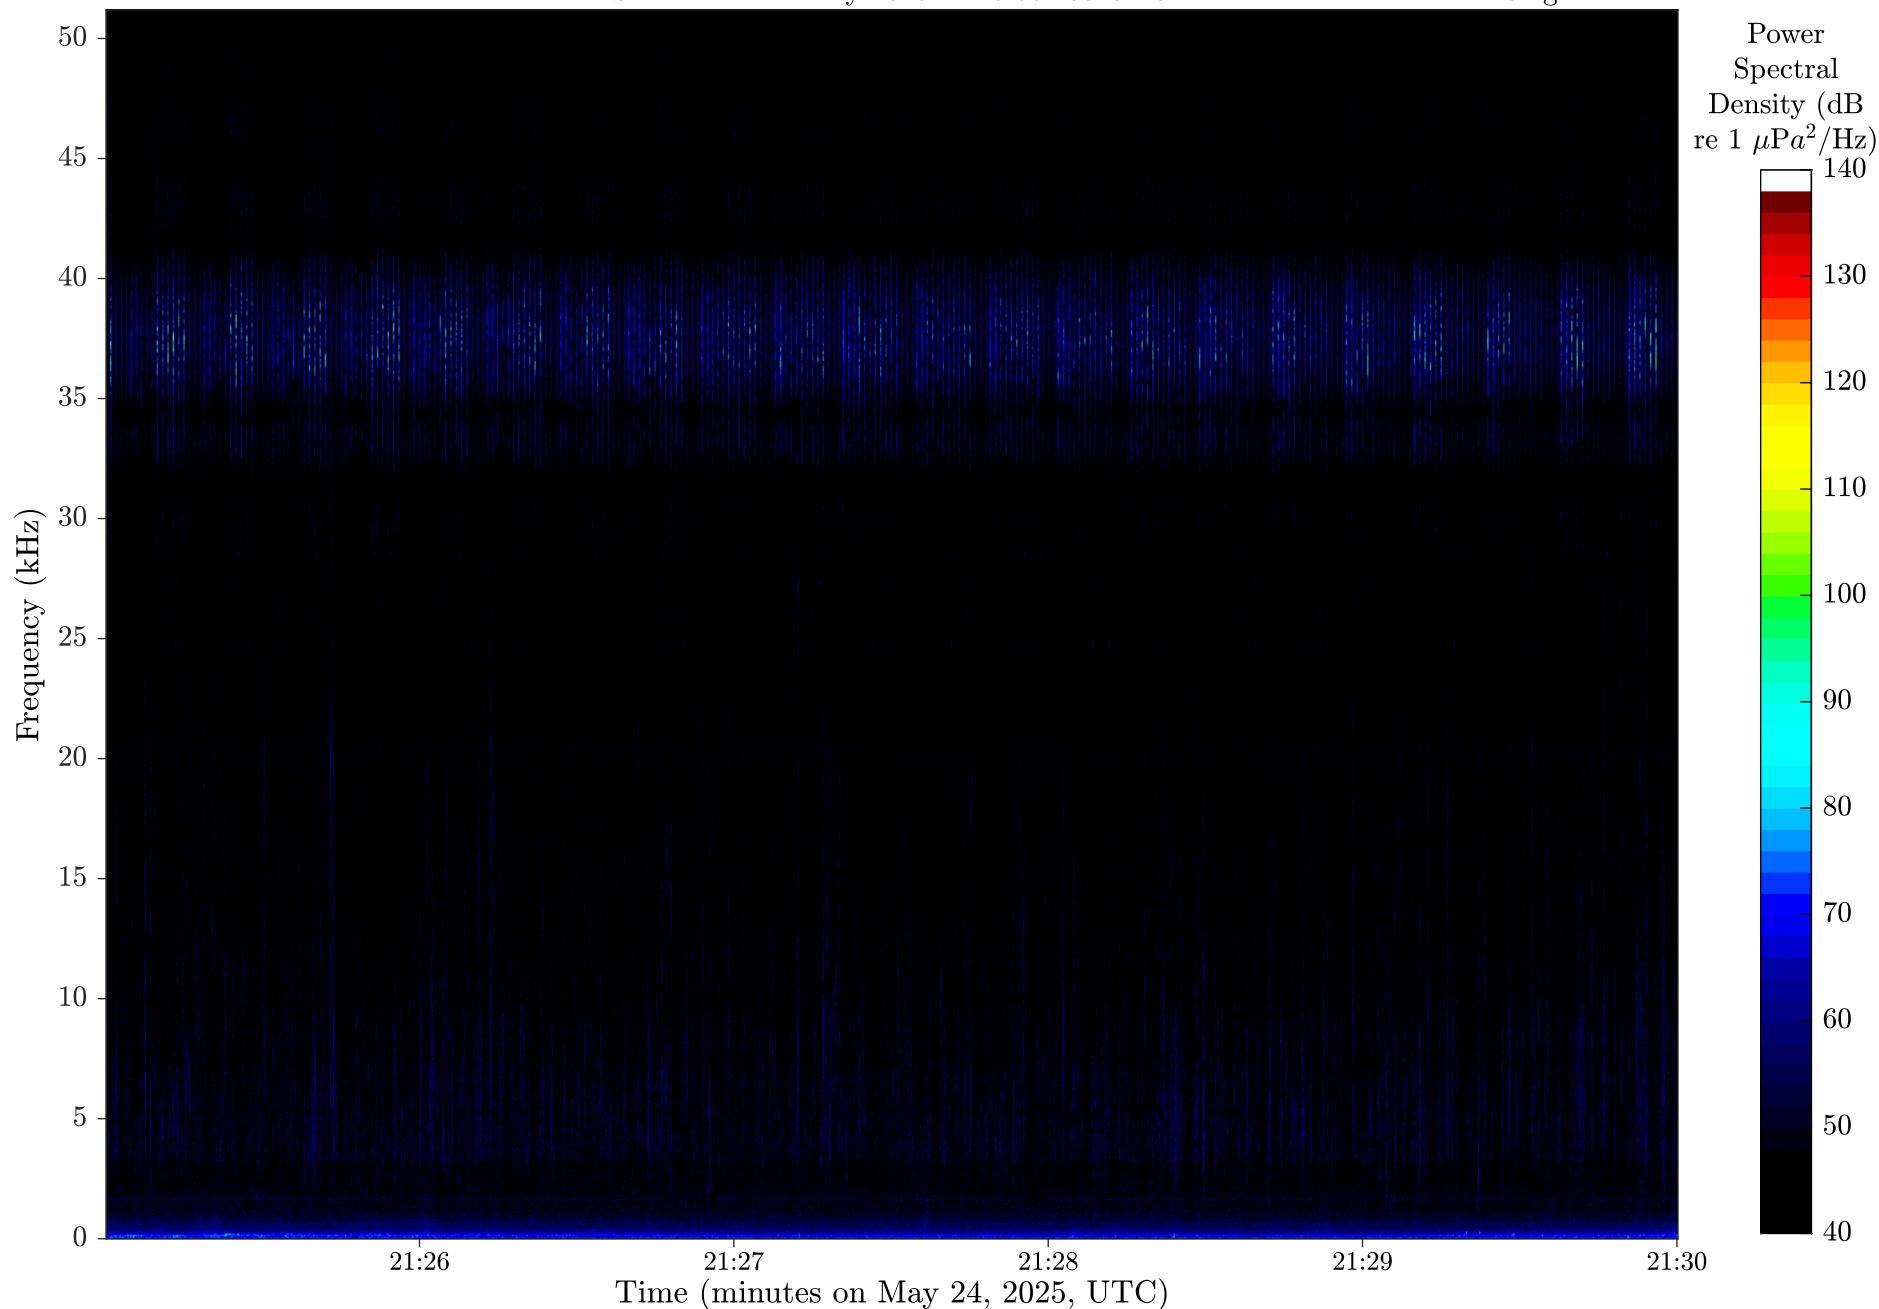

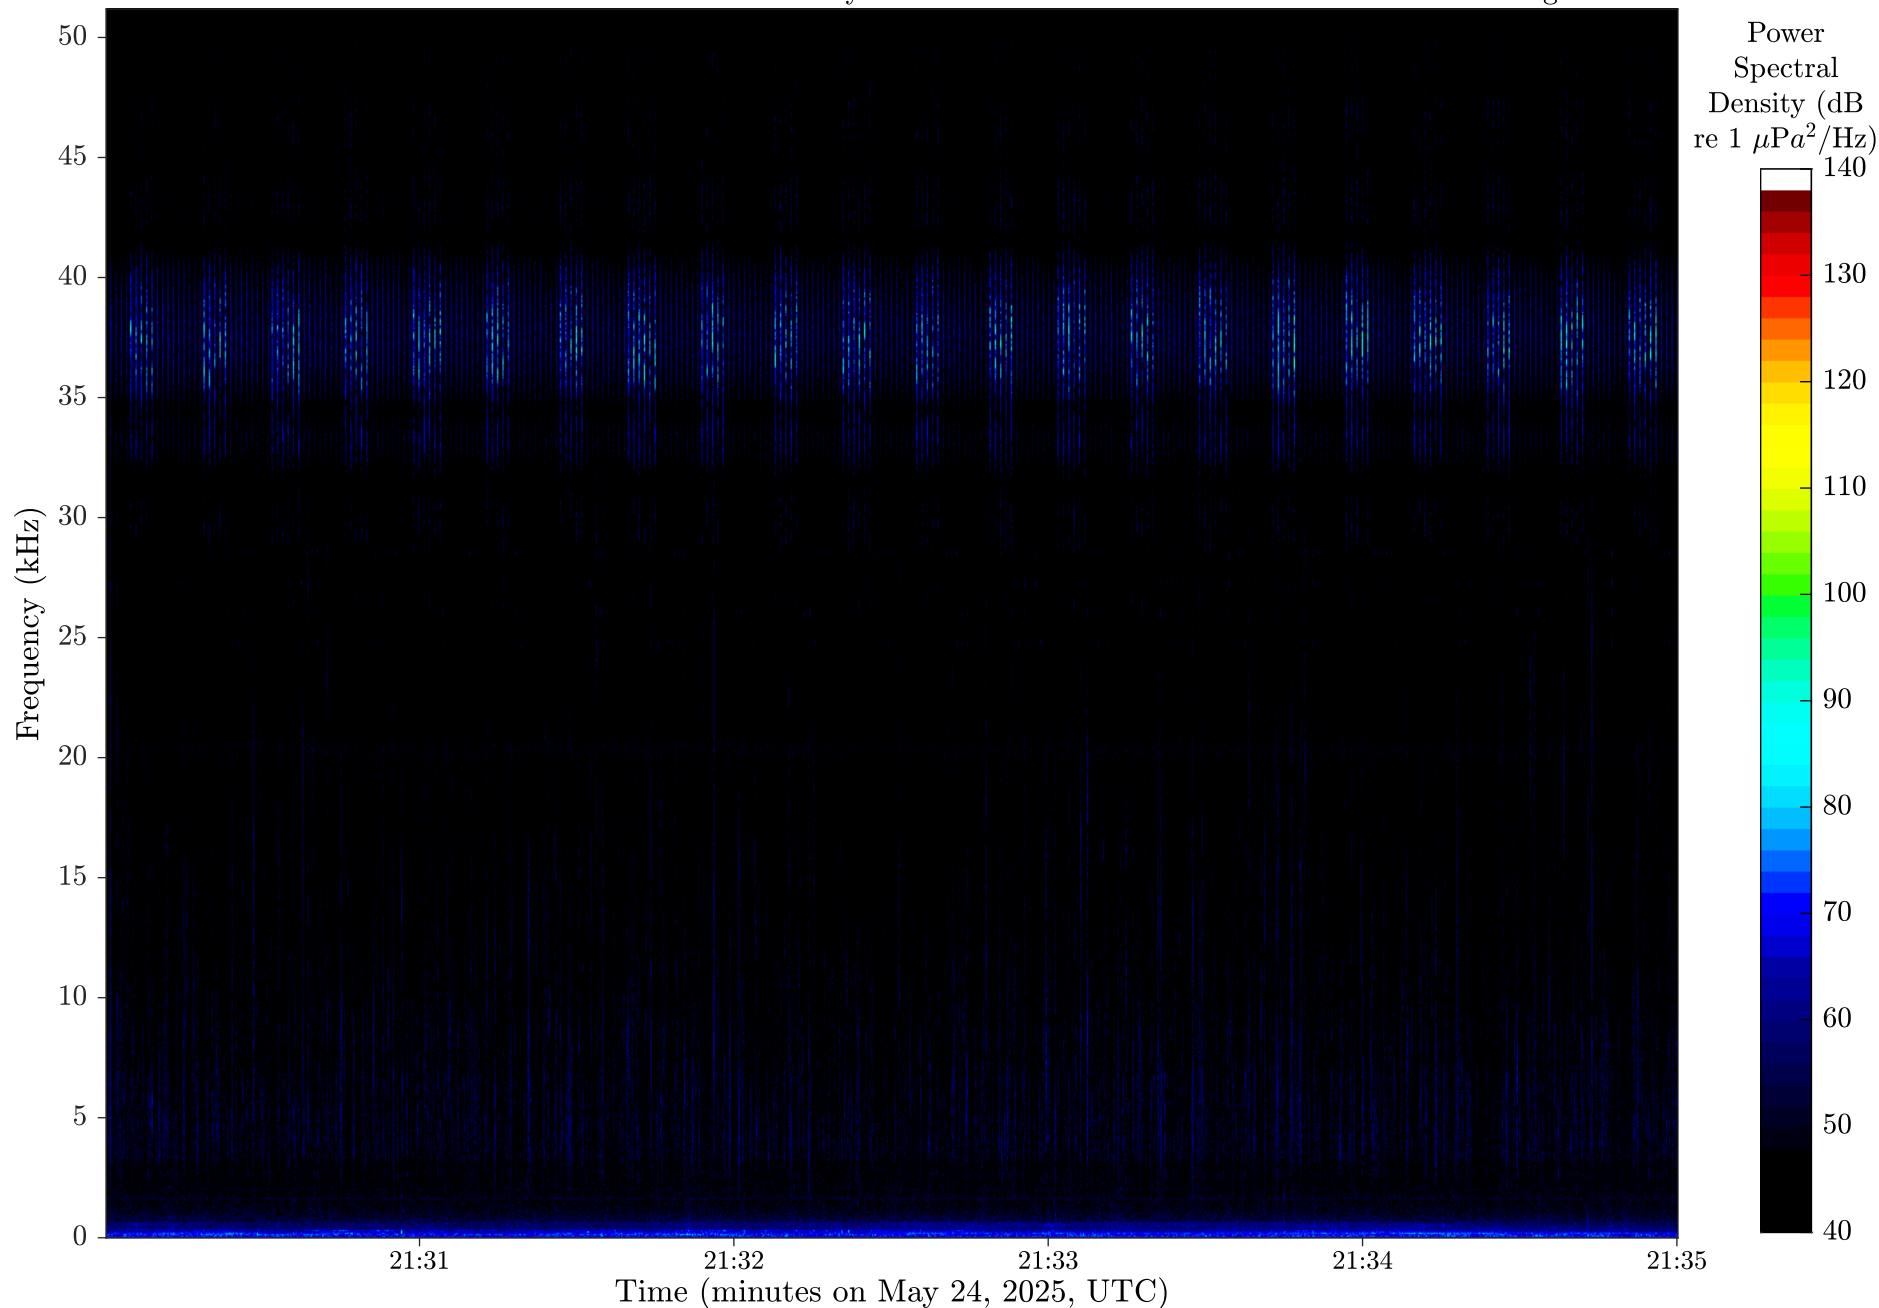


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:43:31 UTC

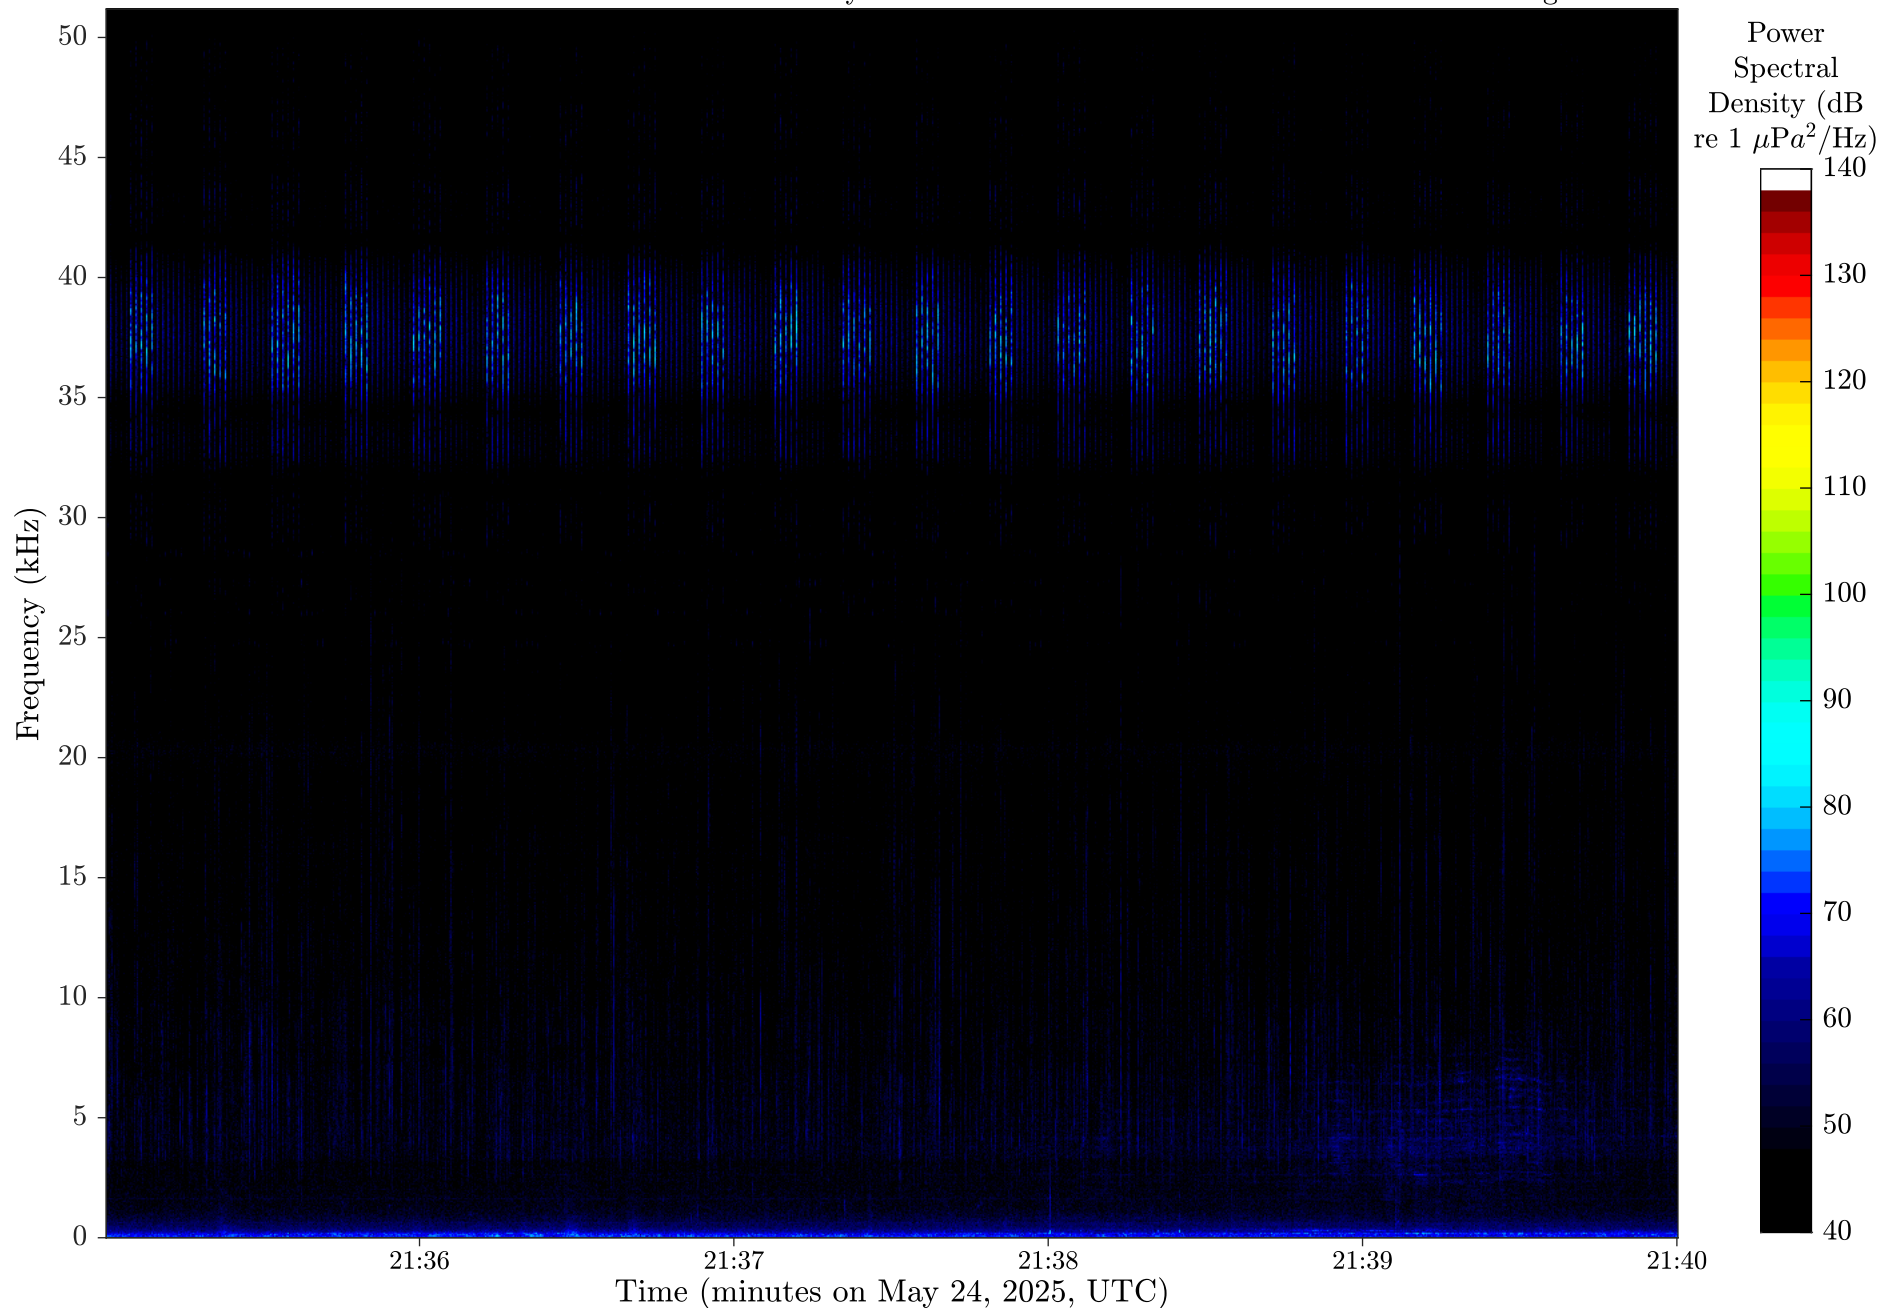


Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:43:39 UTC

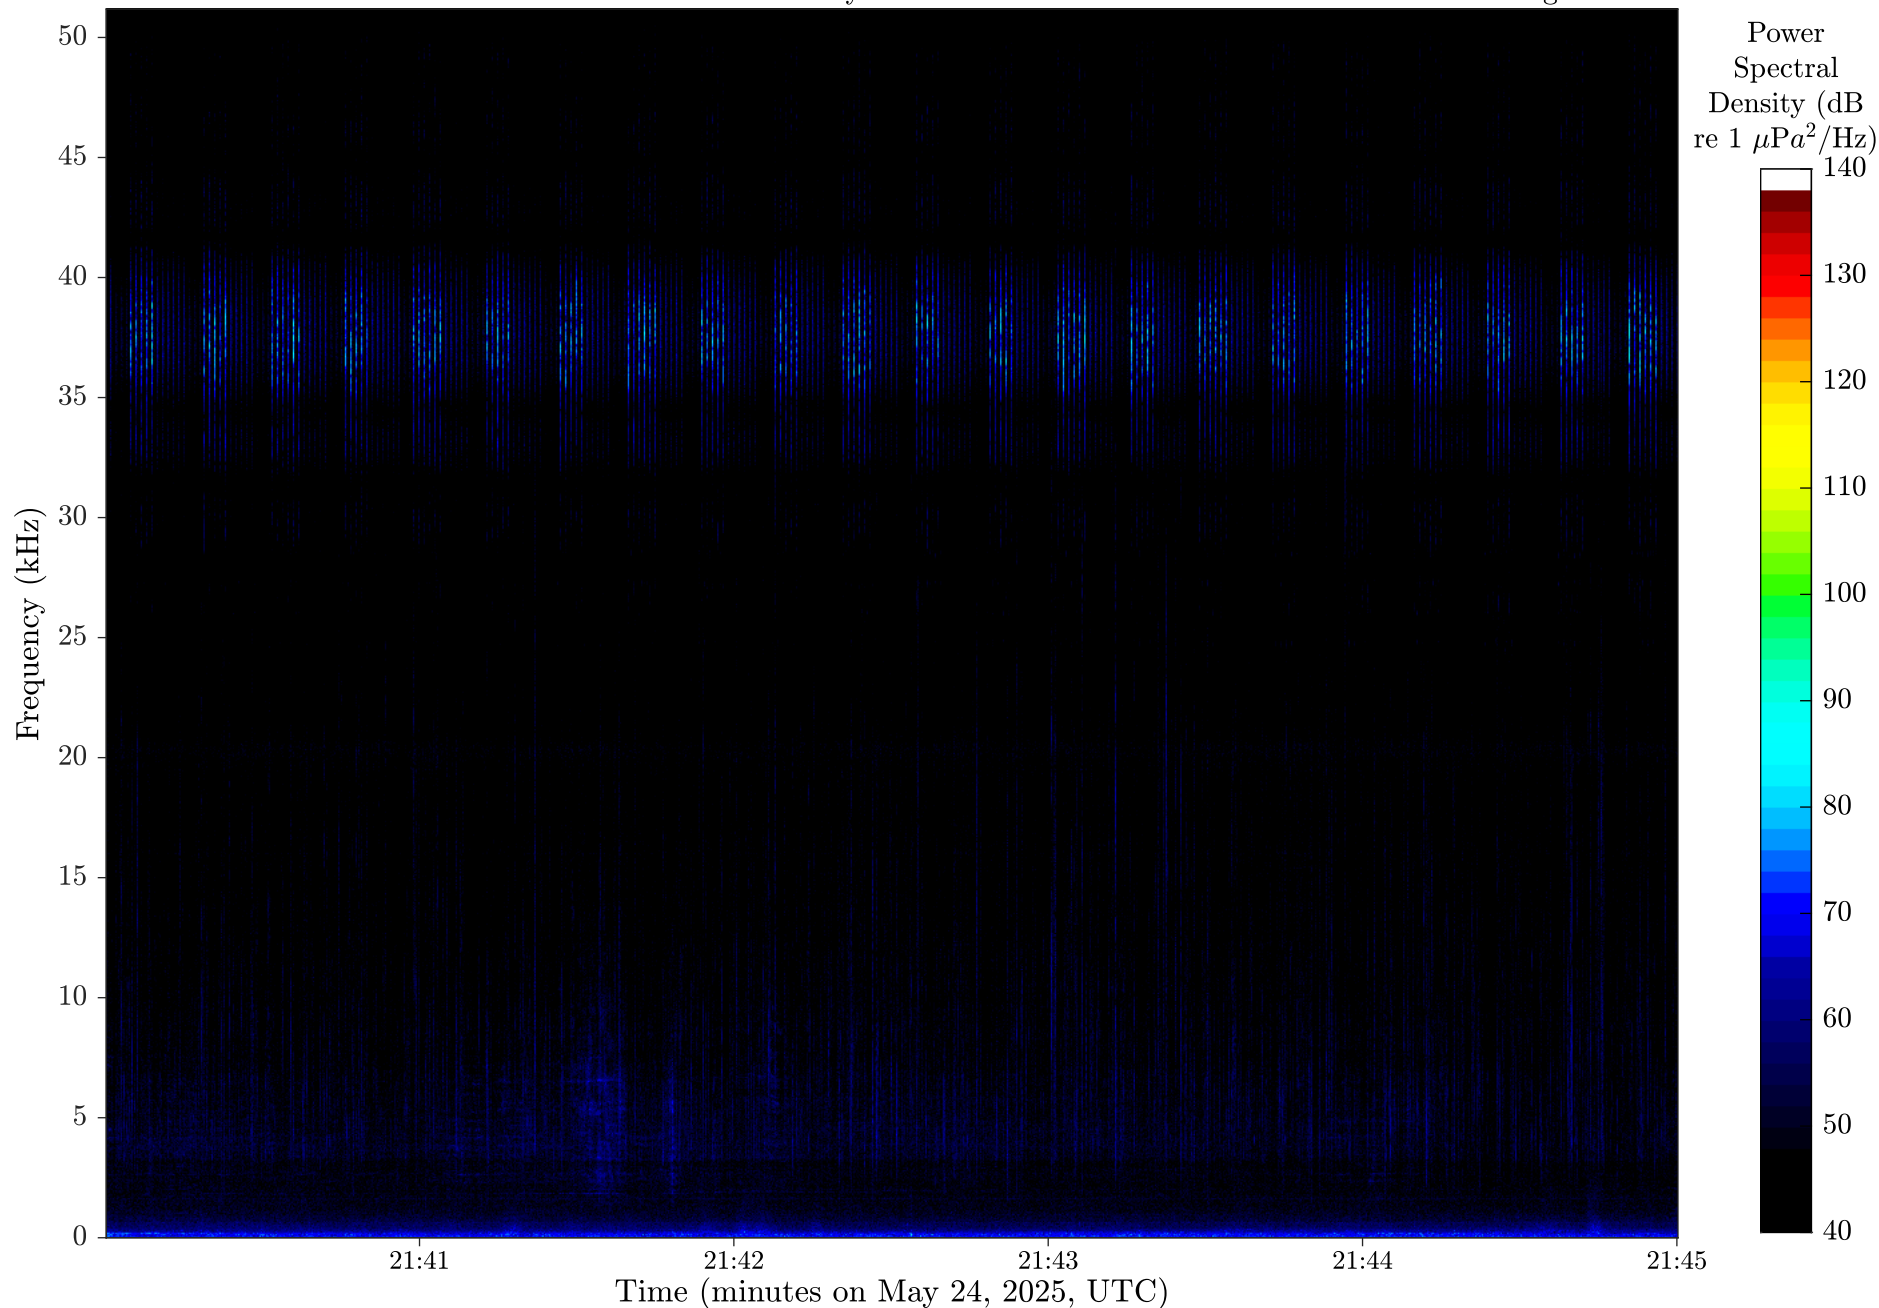



Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:43:46 UTC

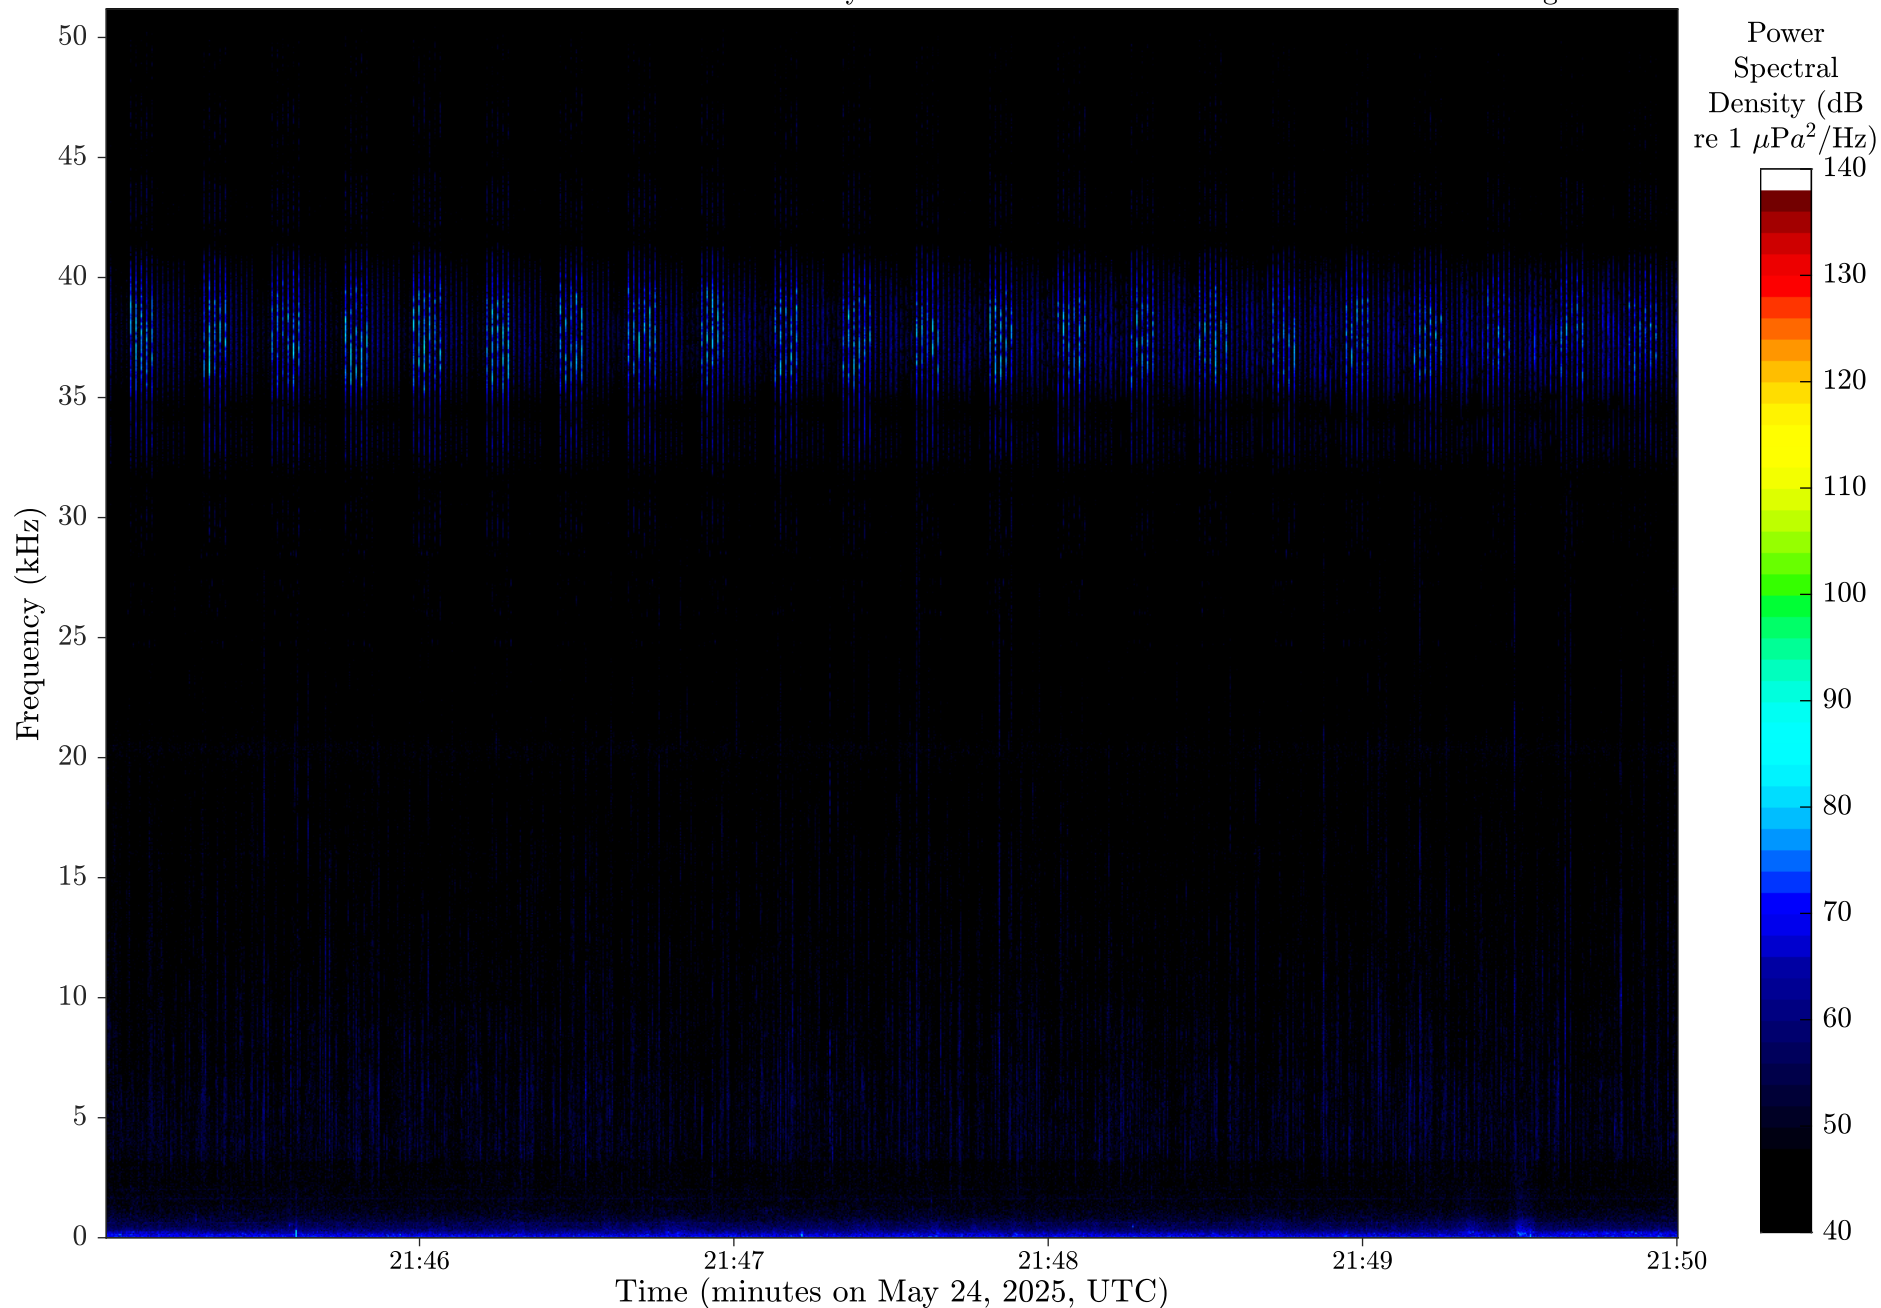

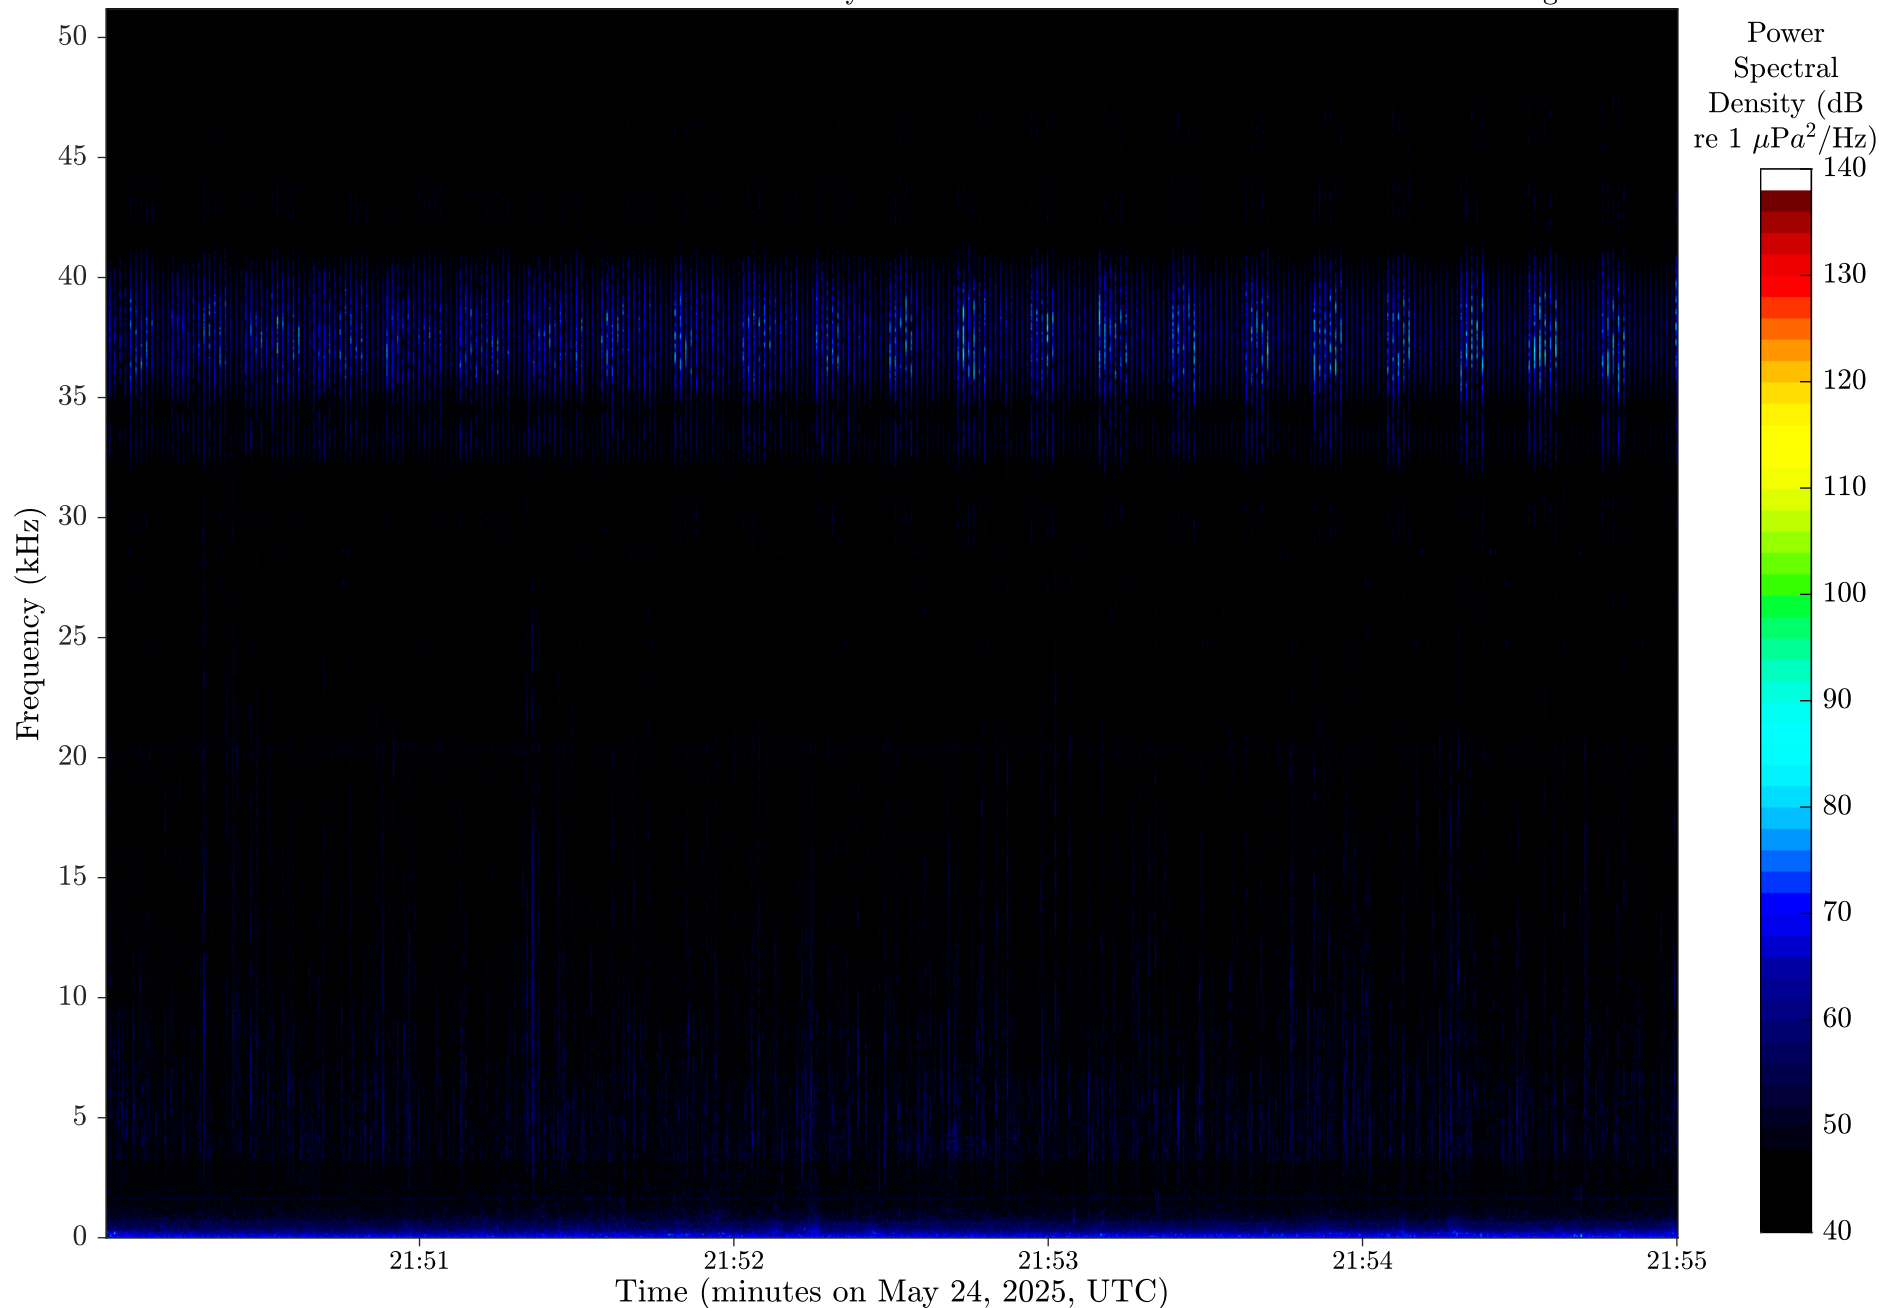


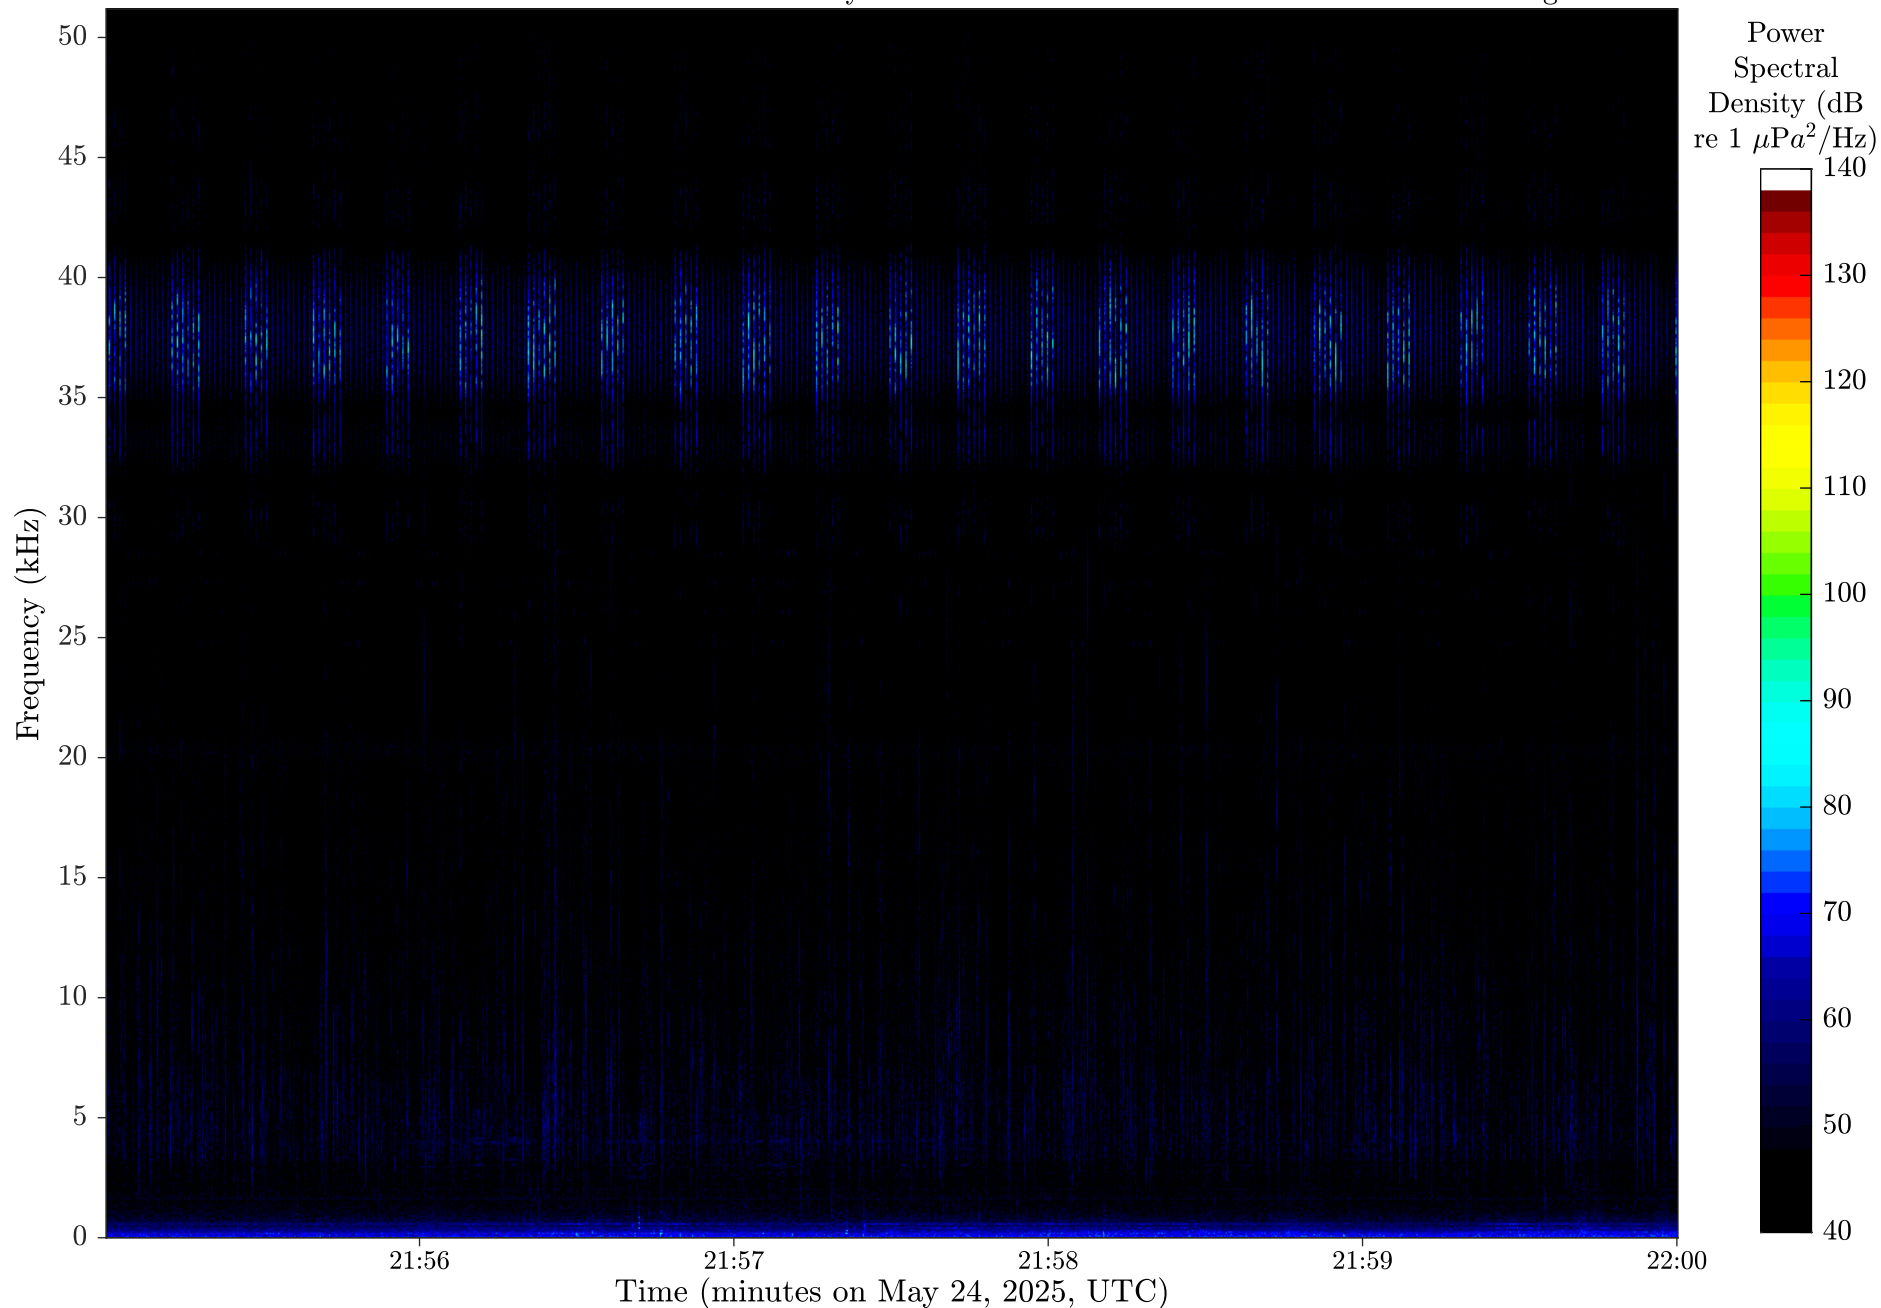

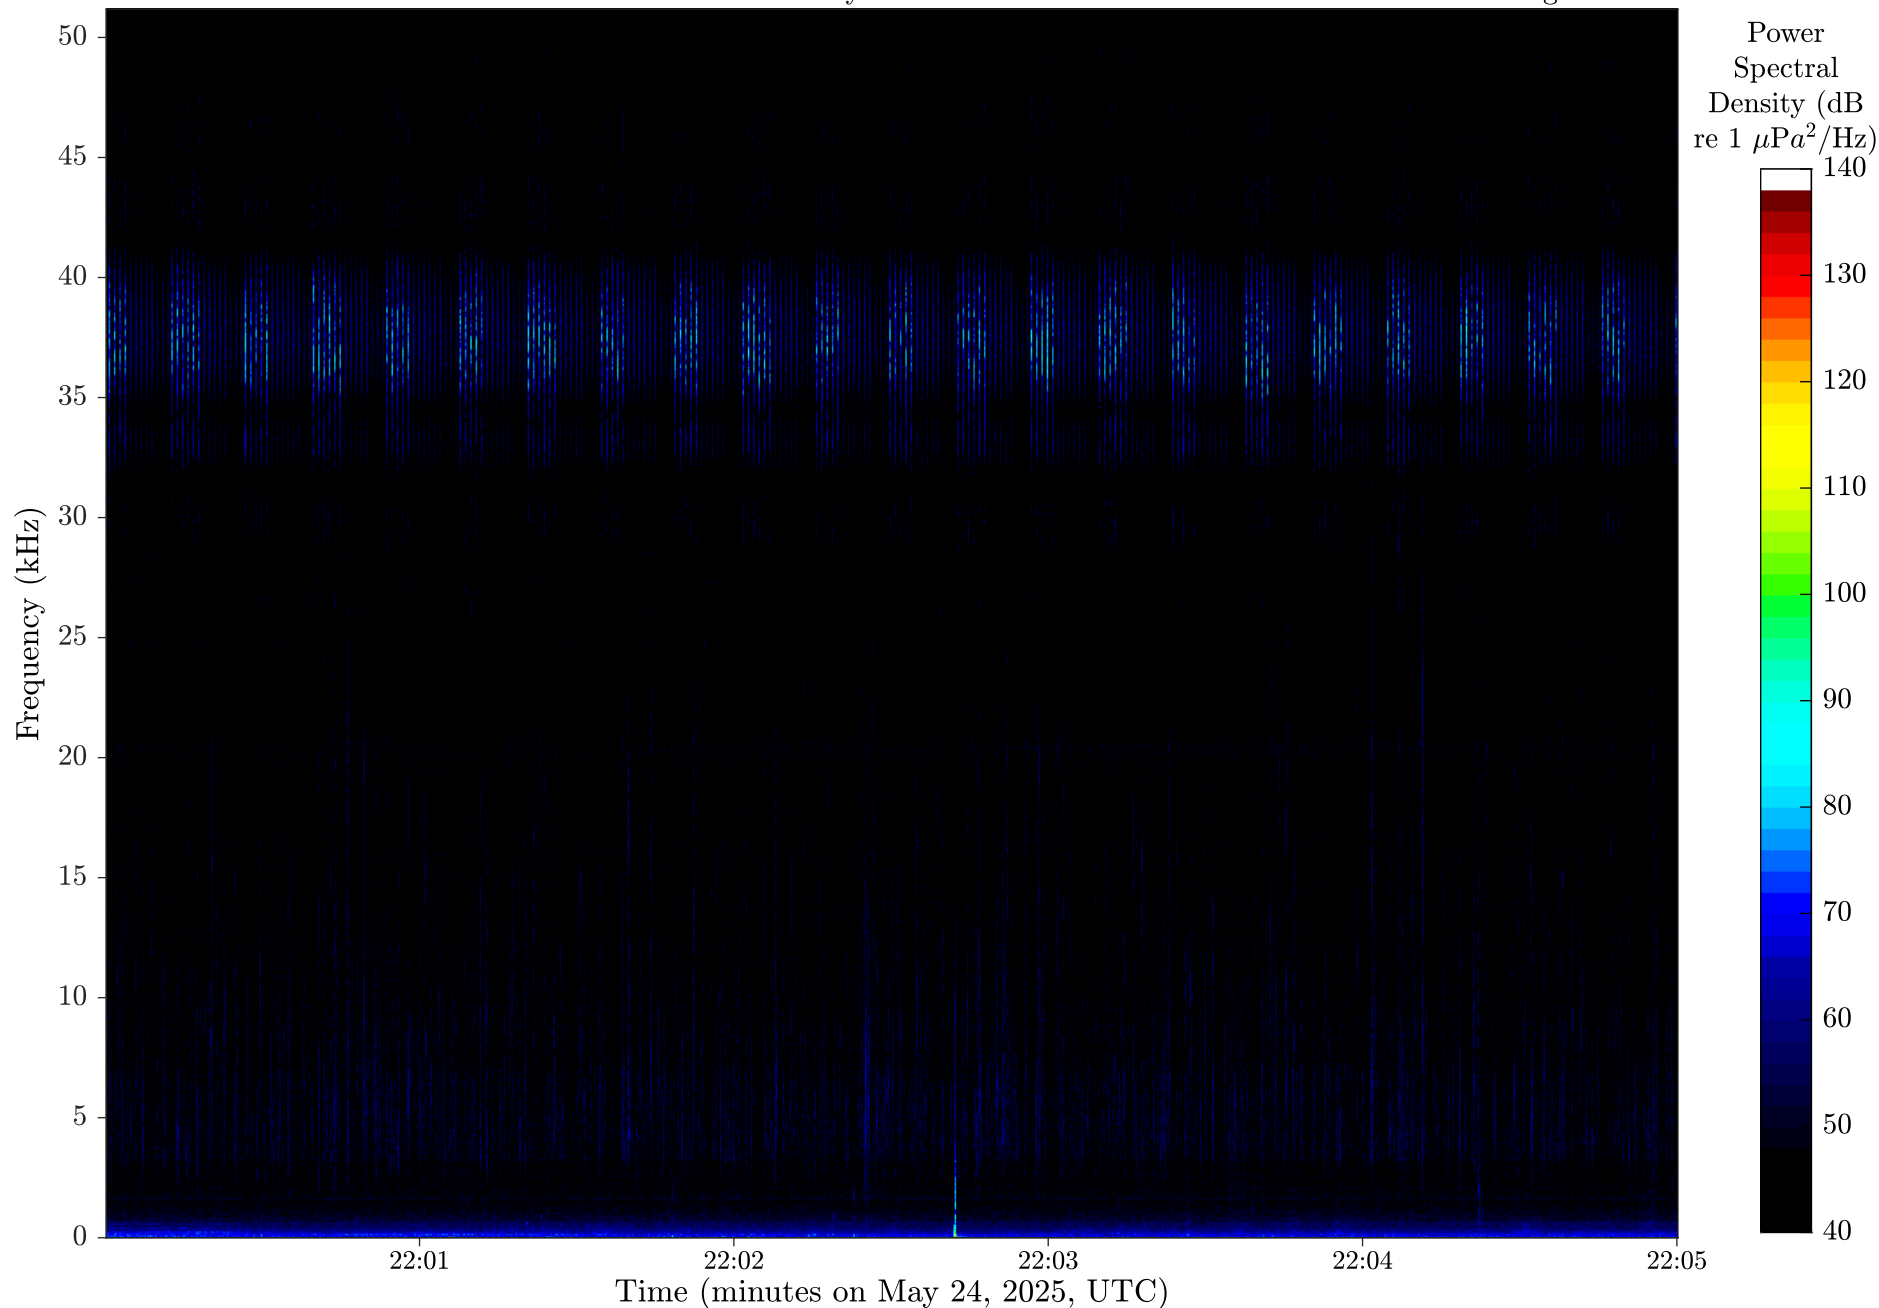


Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:14 UTC

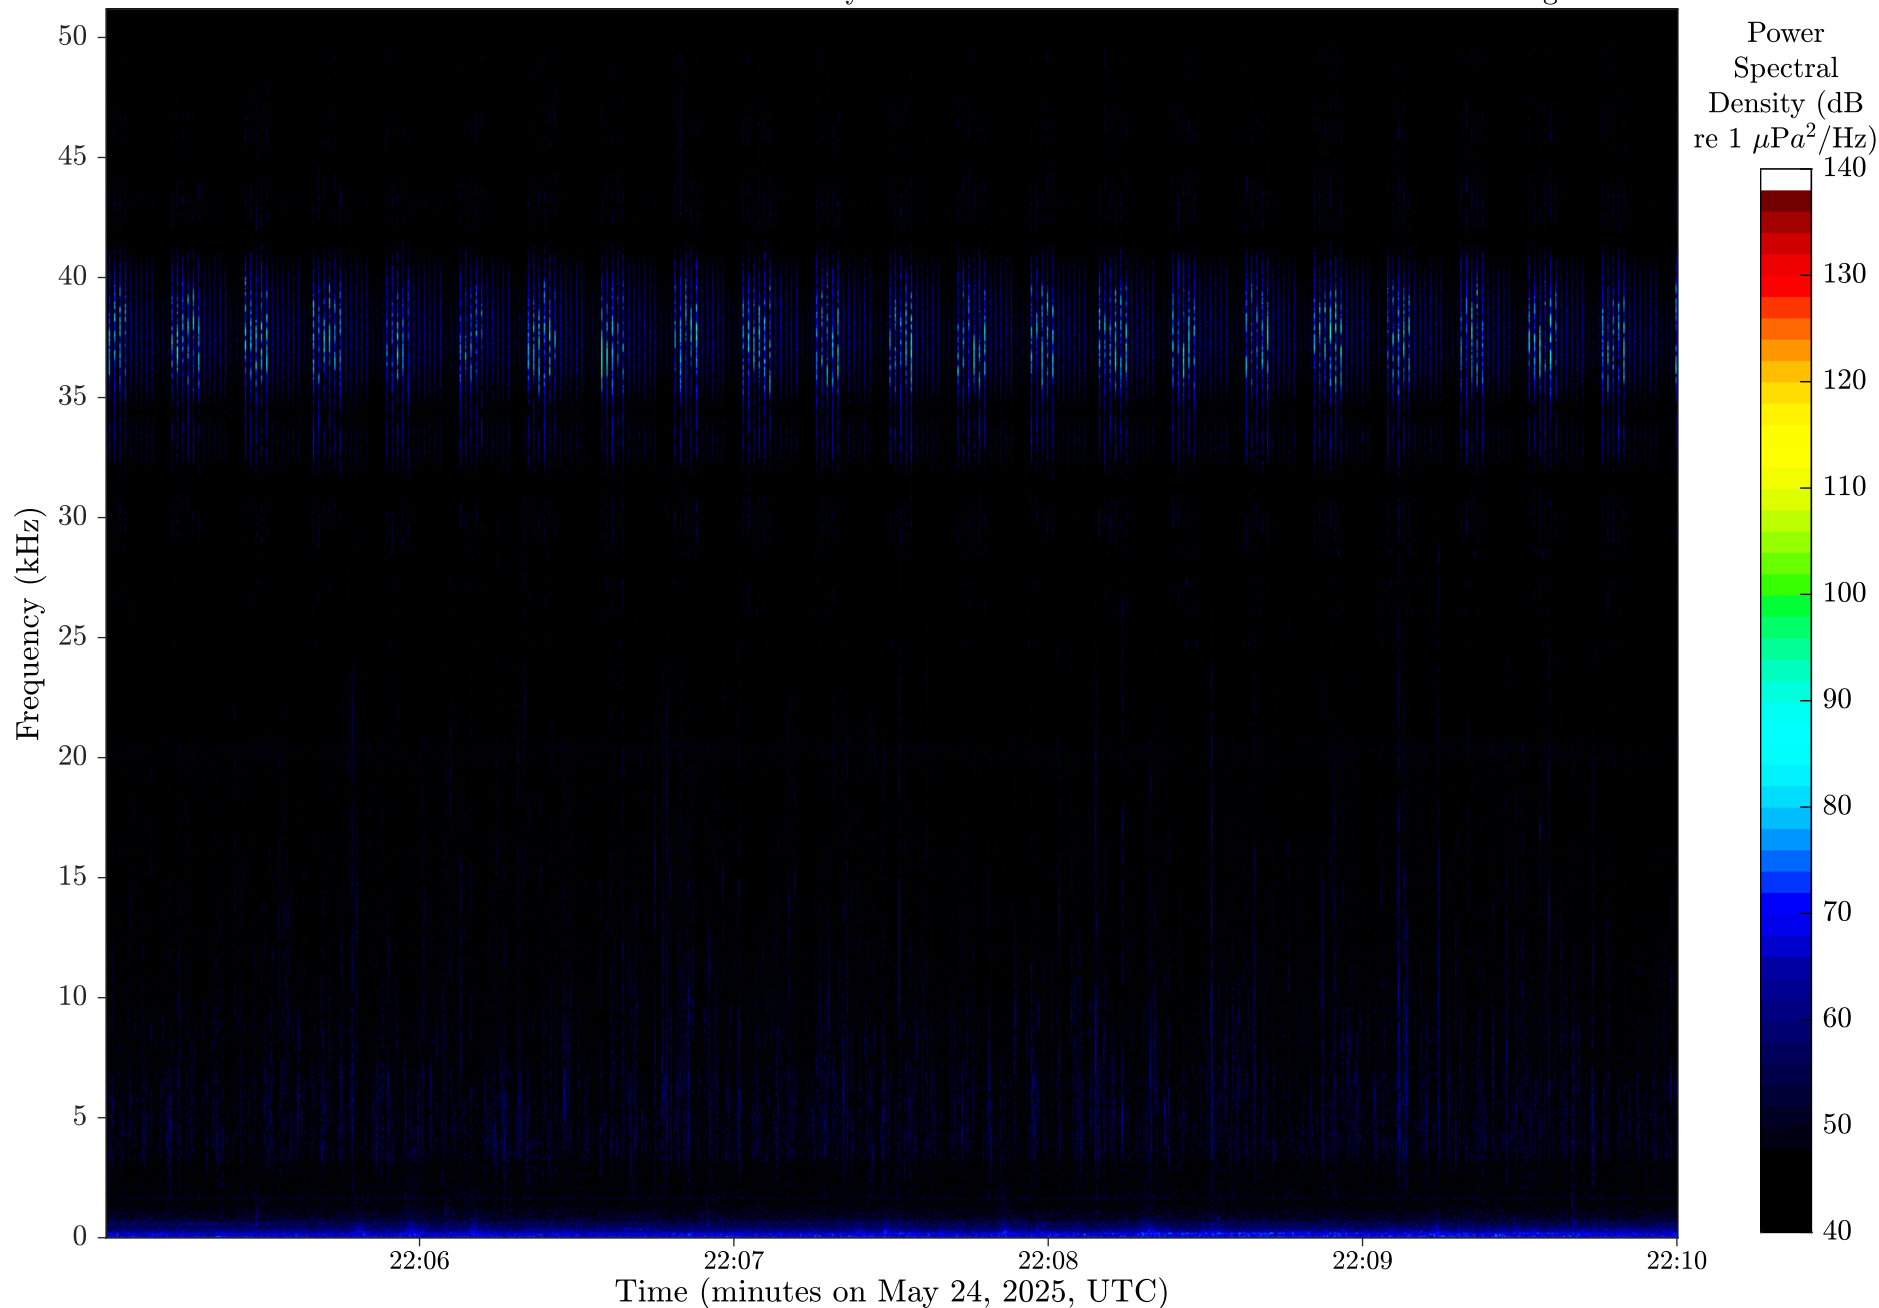


Comments: 34.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:21 UTC

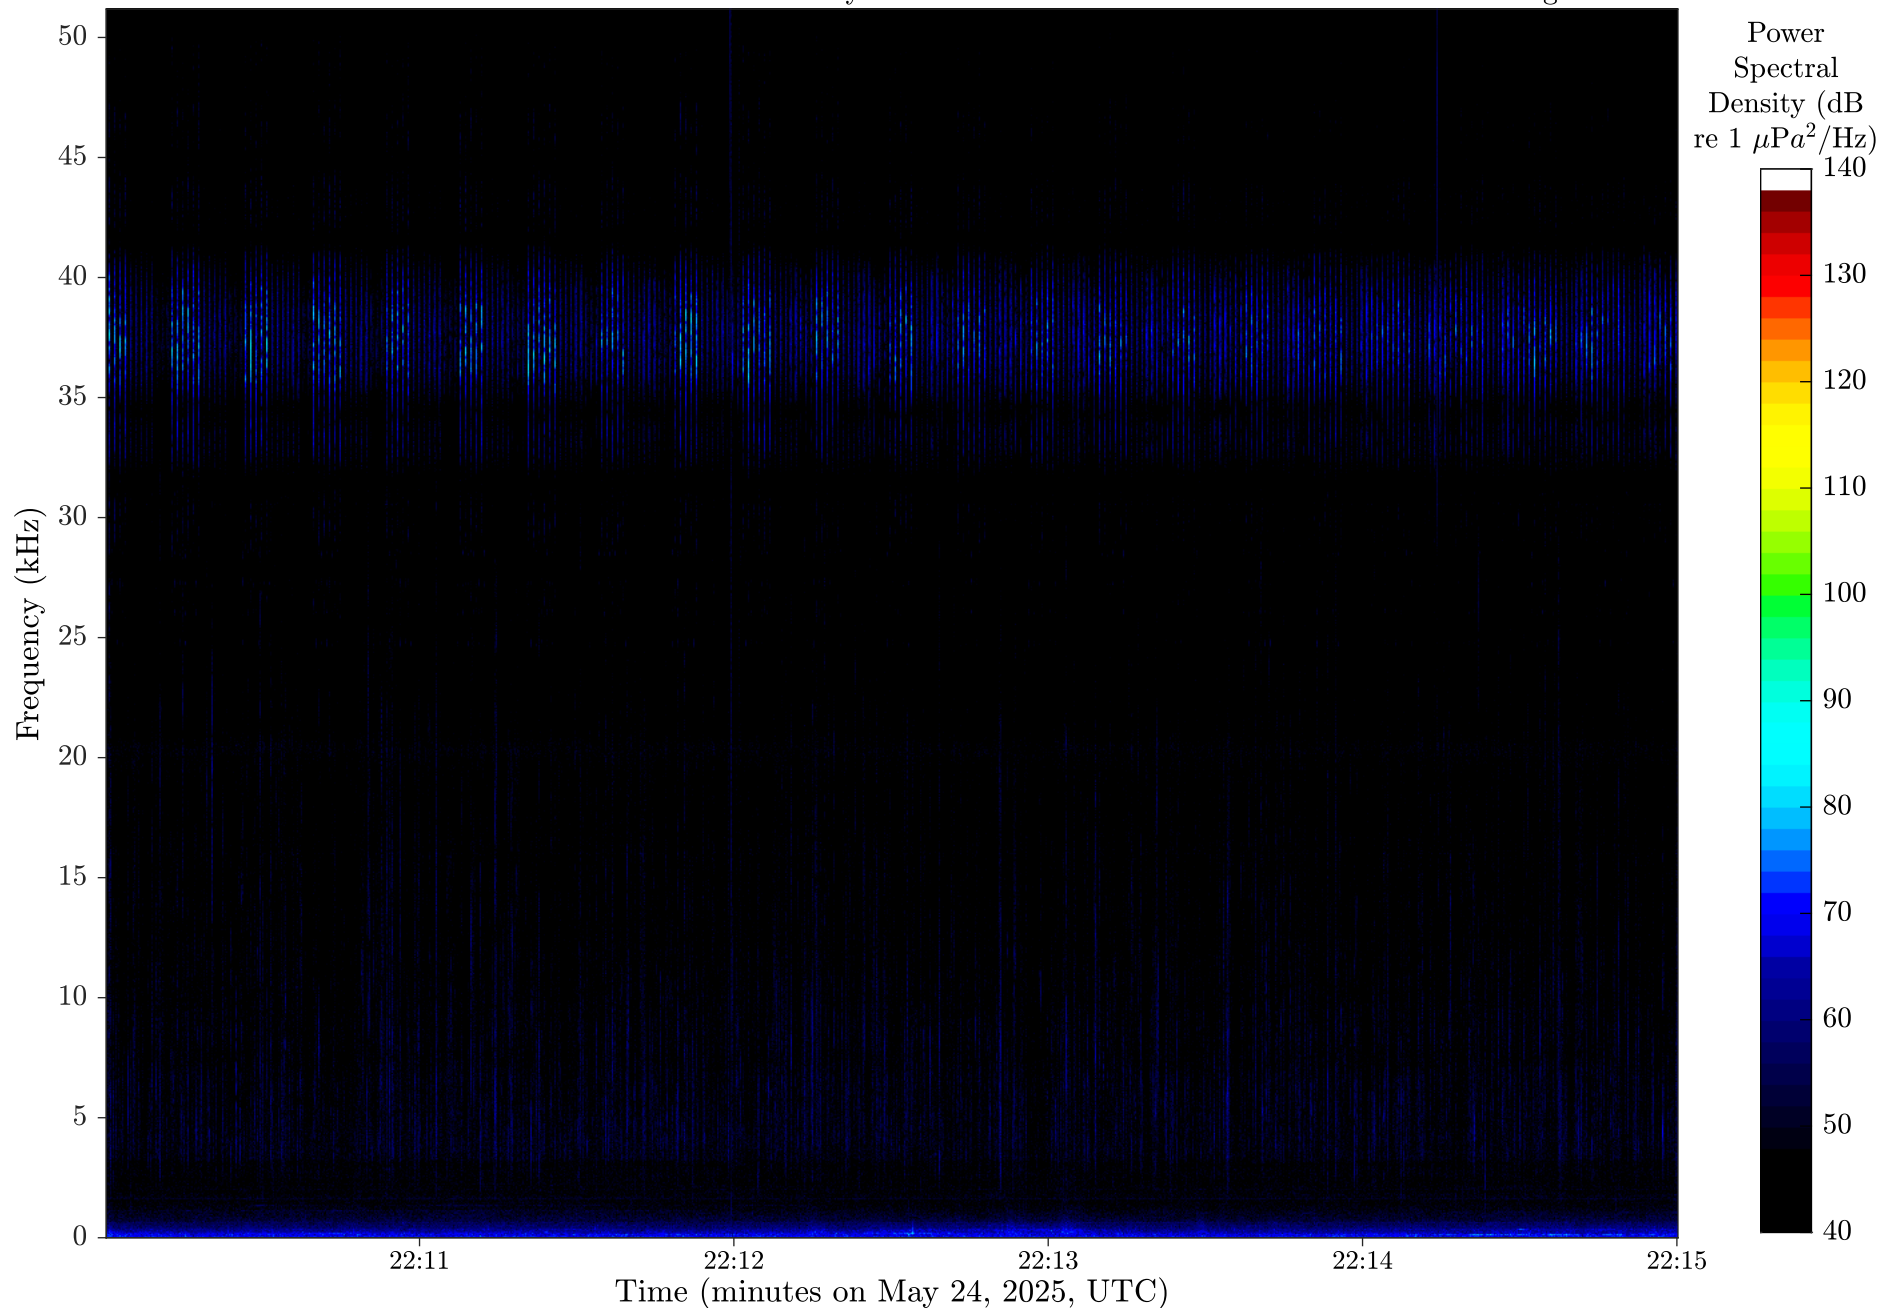


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:29 UTC

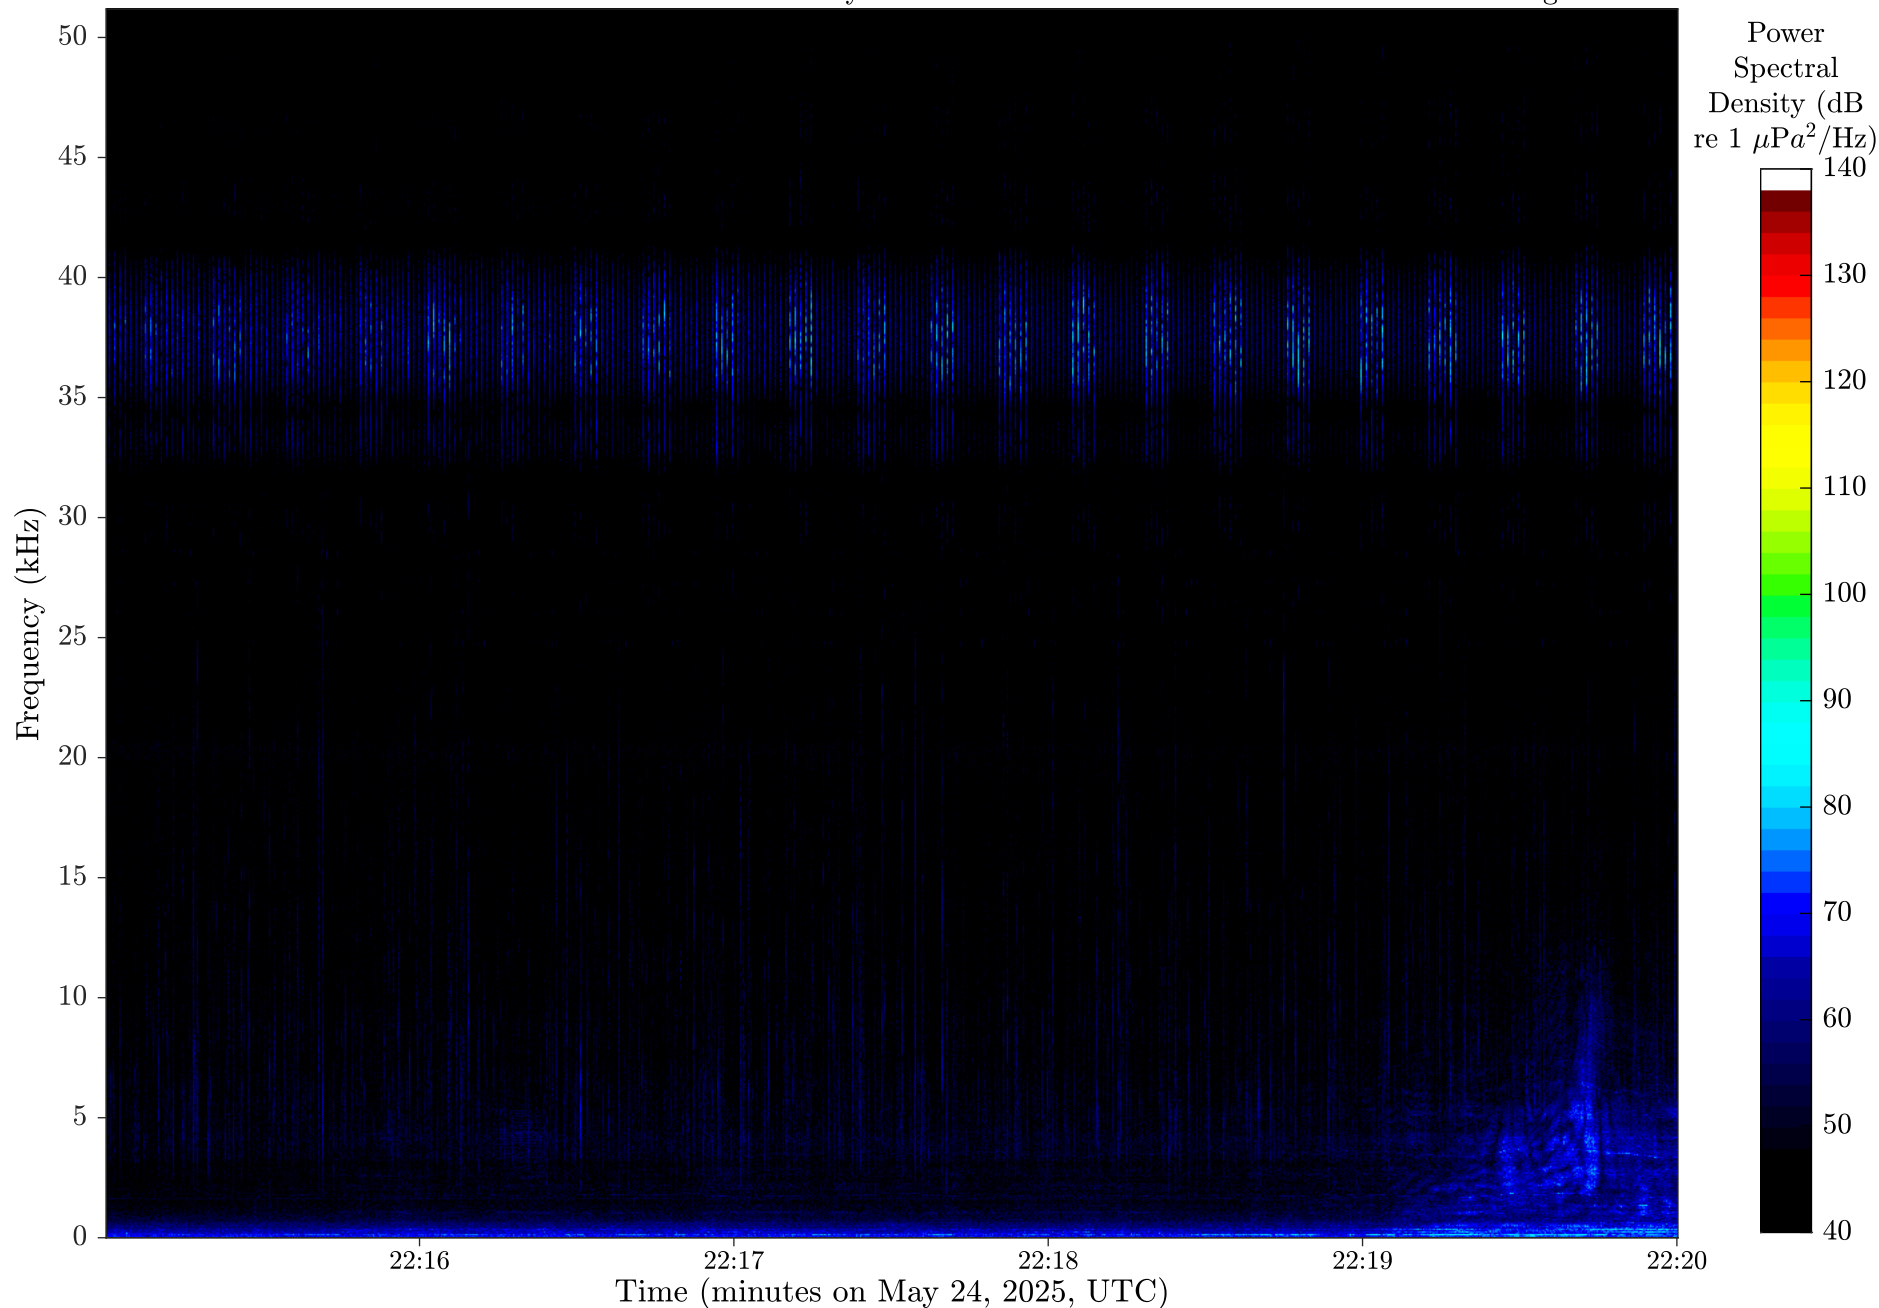


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:36 UTC

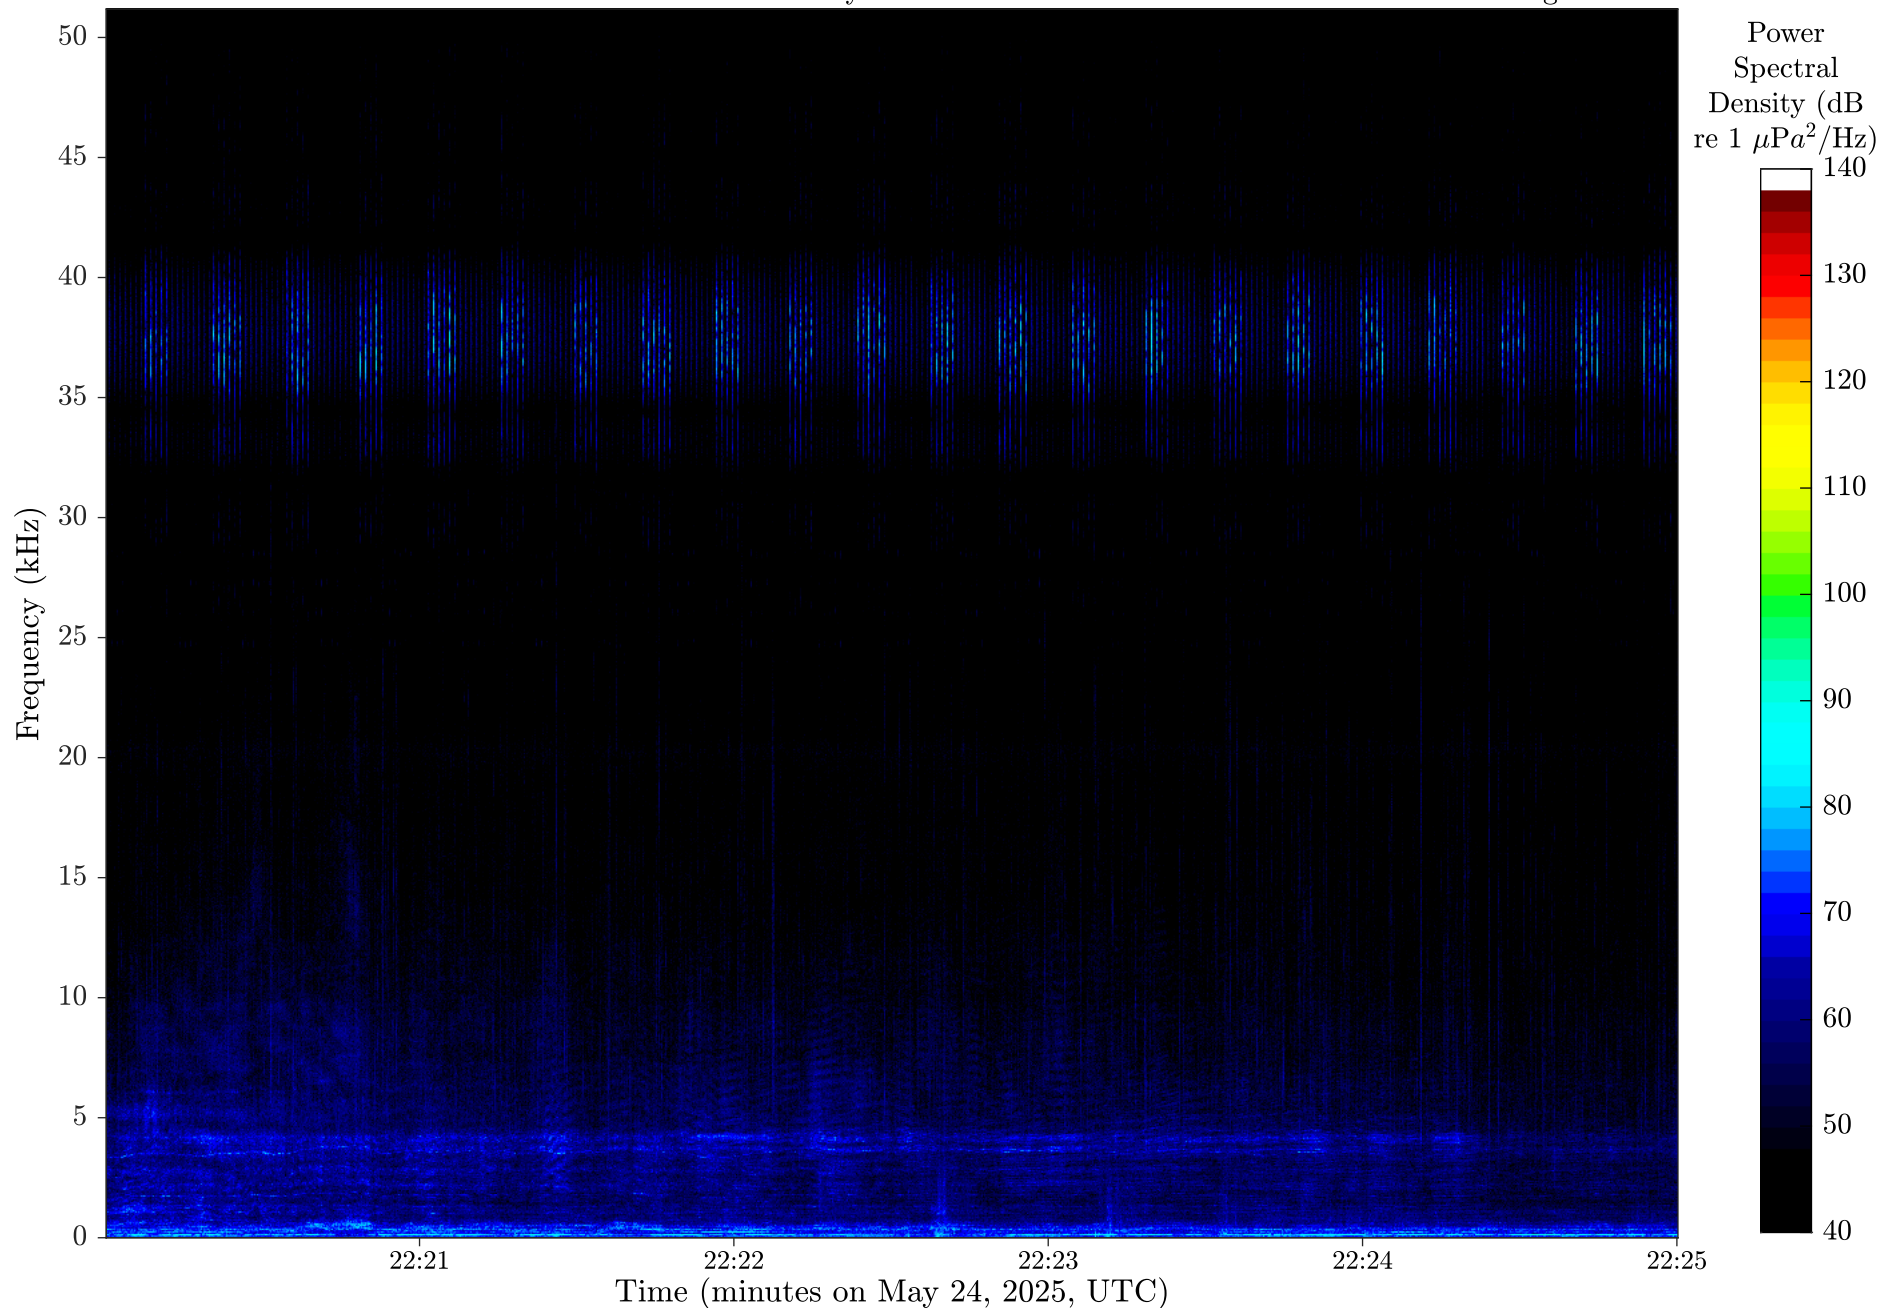


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:43 UTC

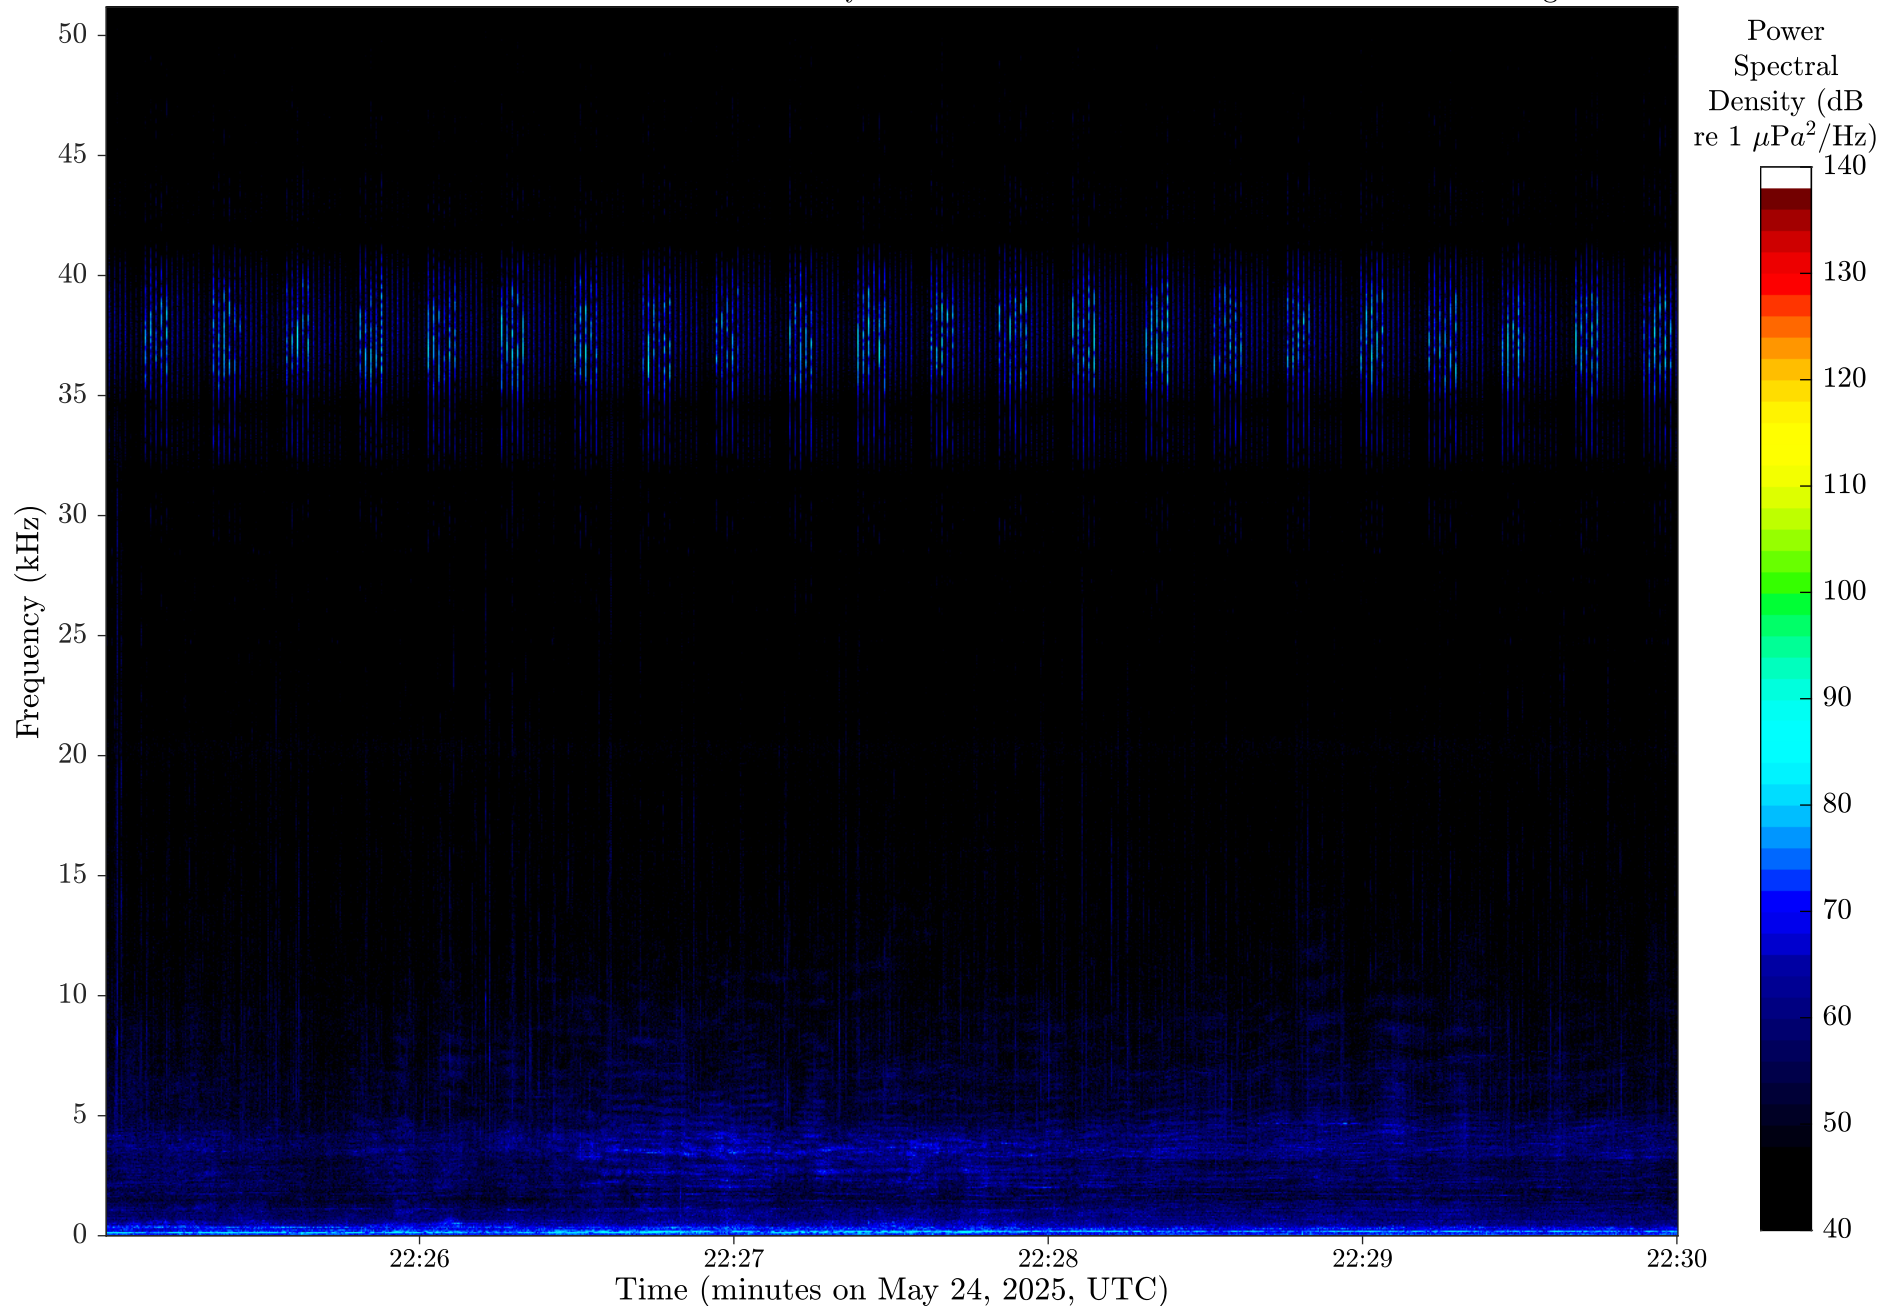


Comments: 34.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:44:50 UTC

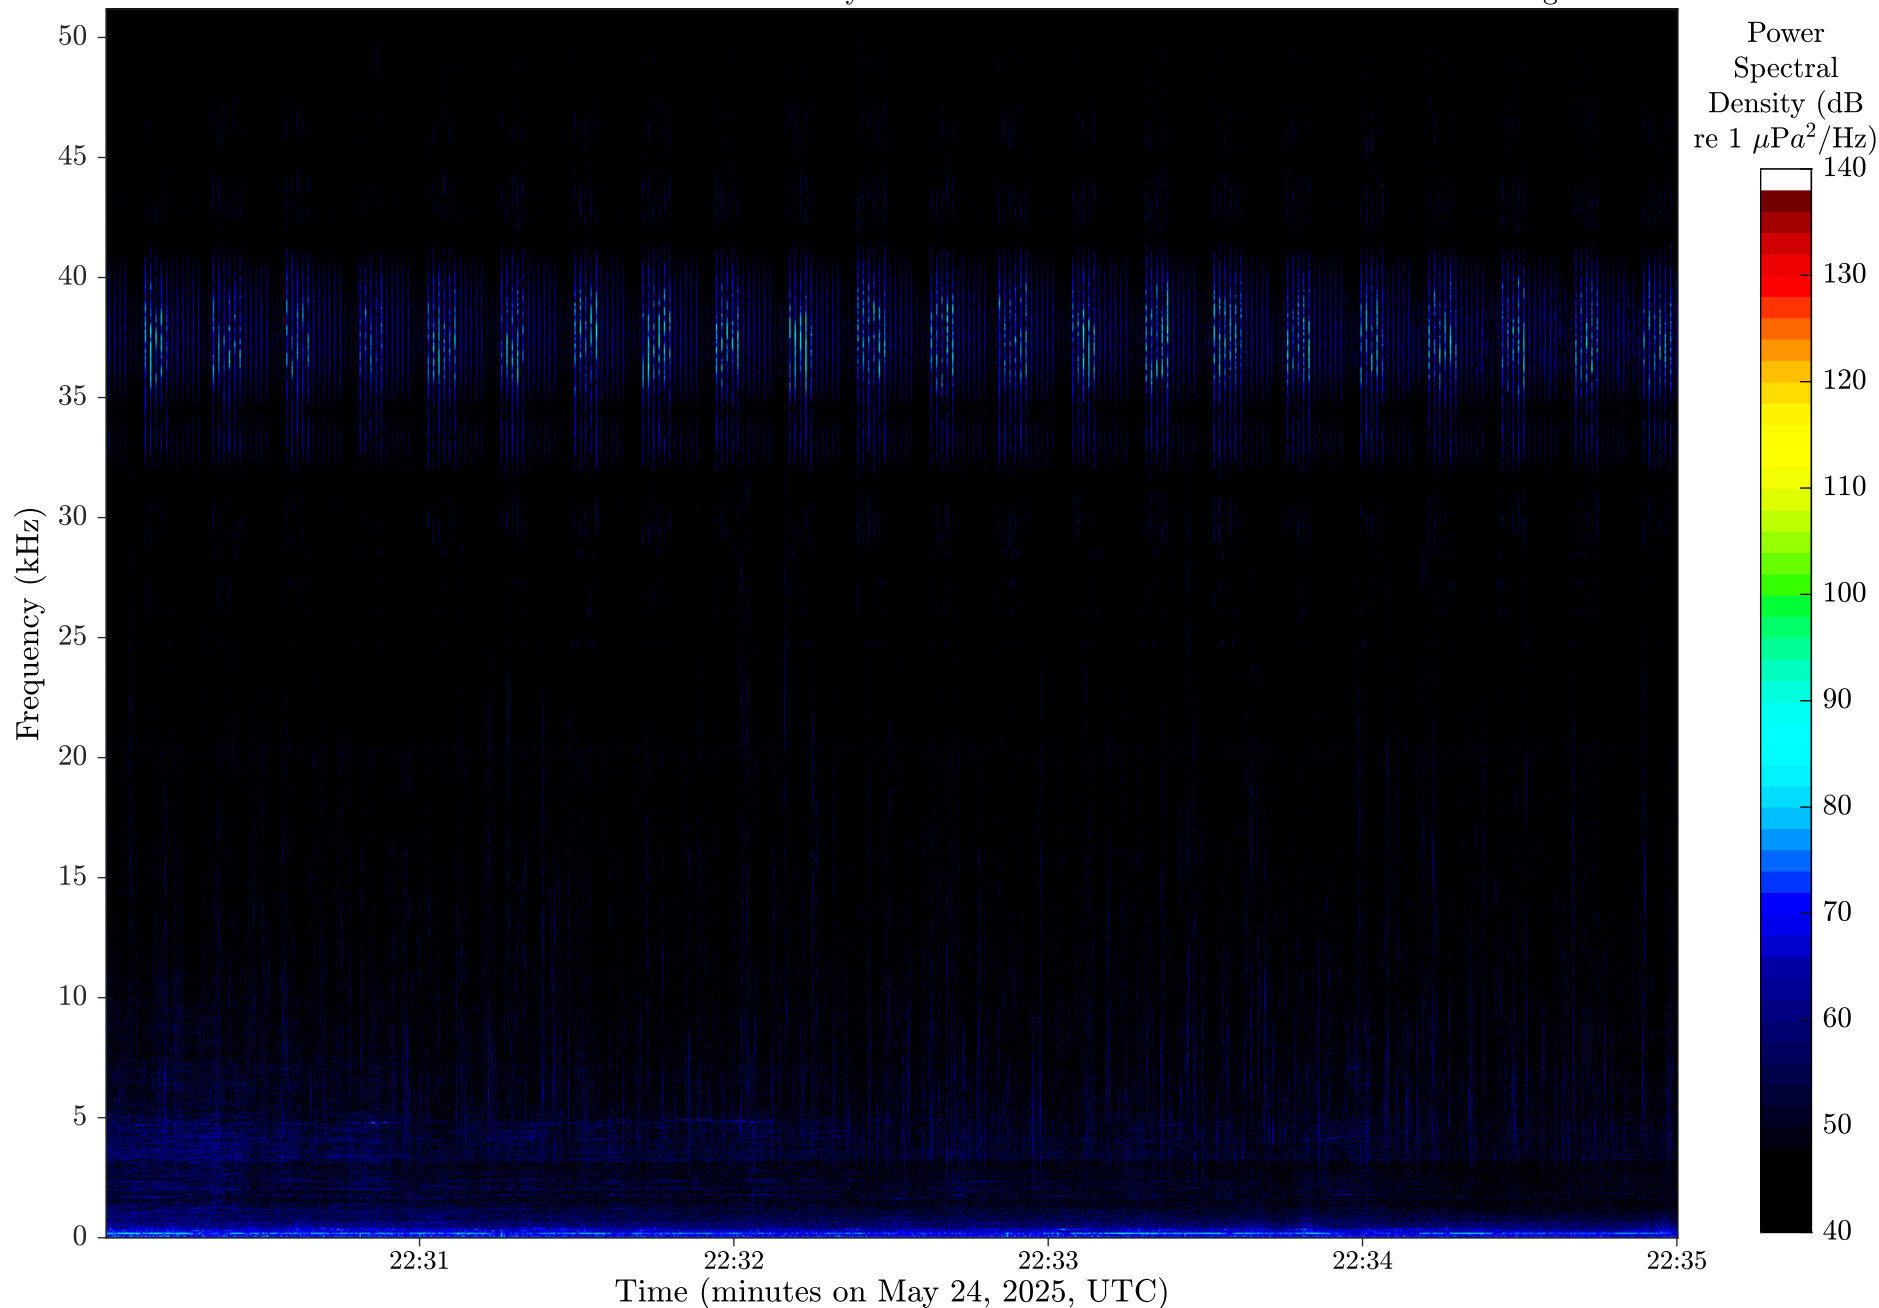


Comments: 34.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:58 UTC

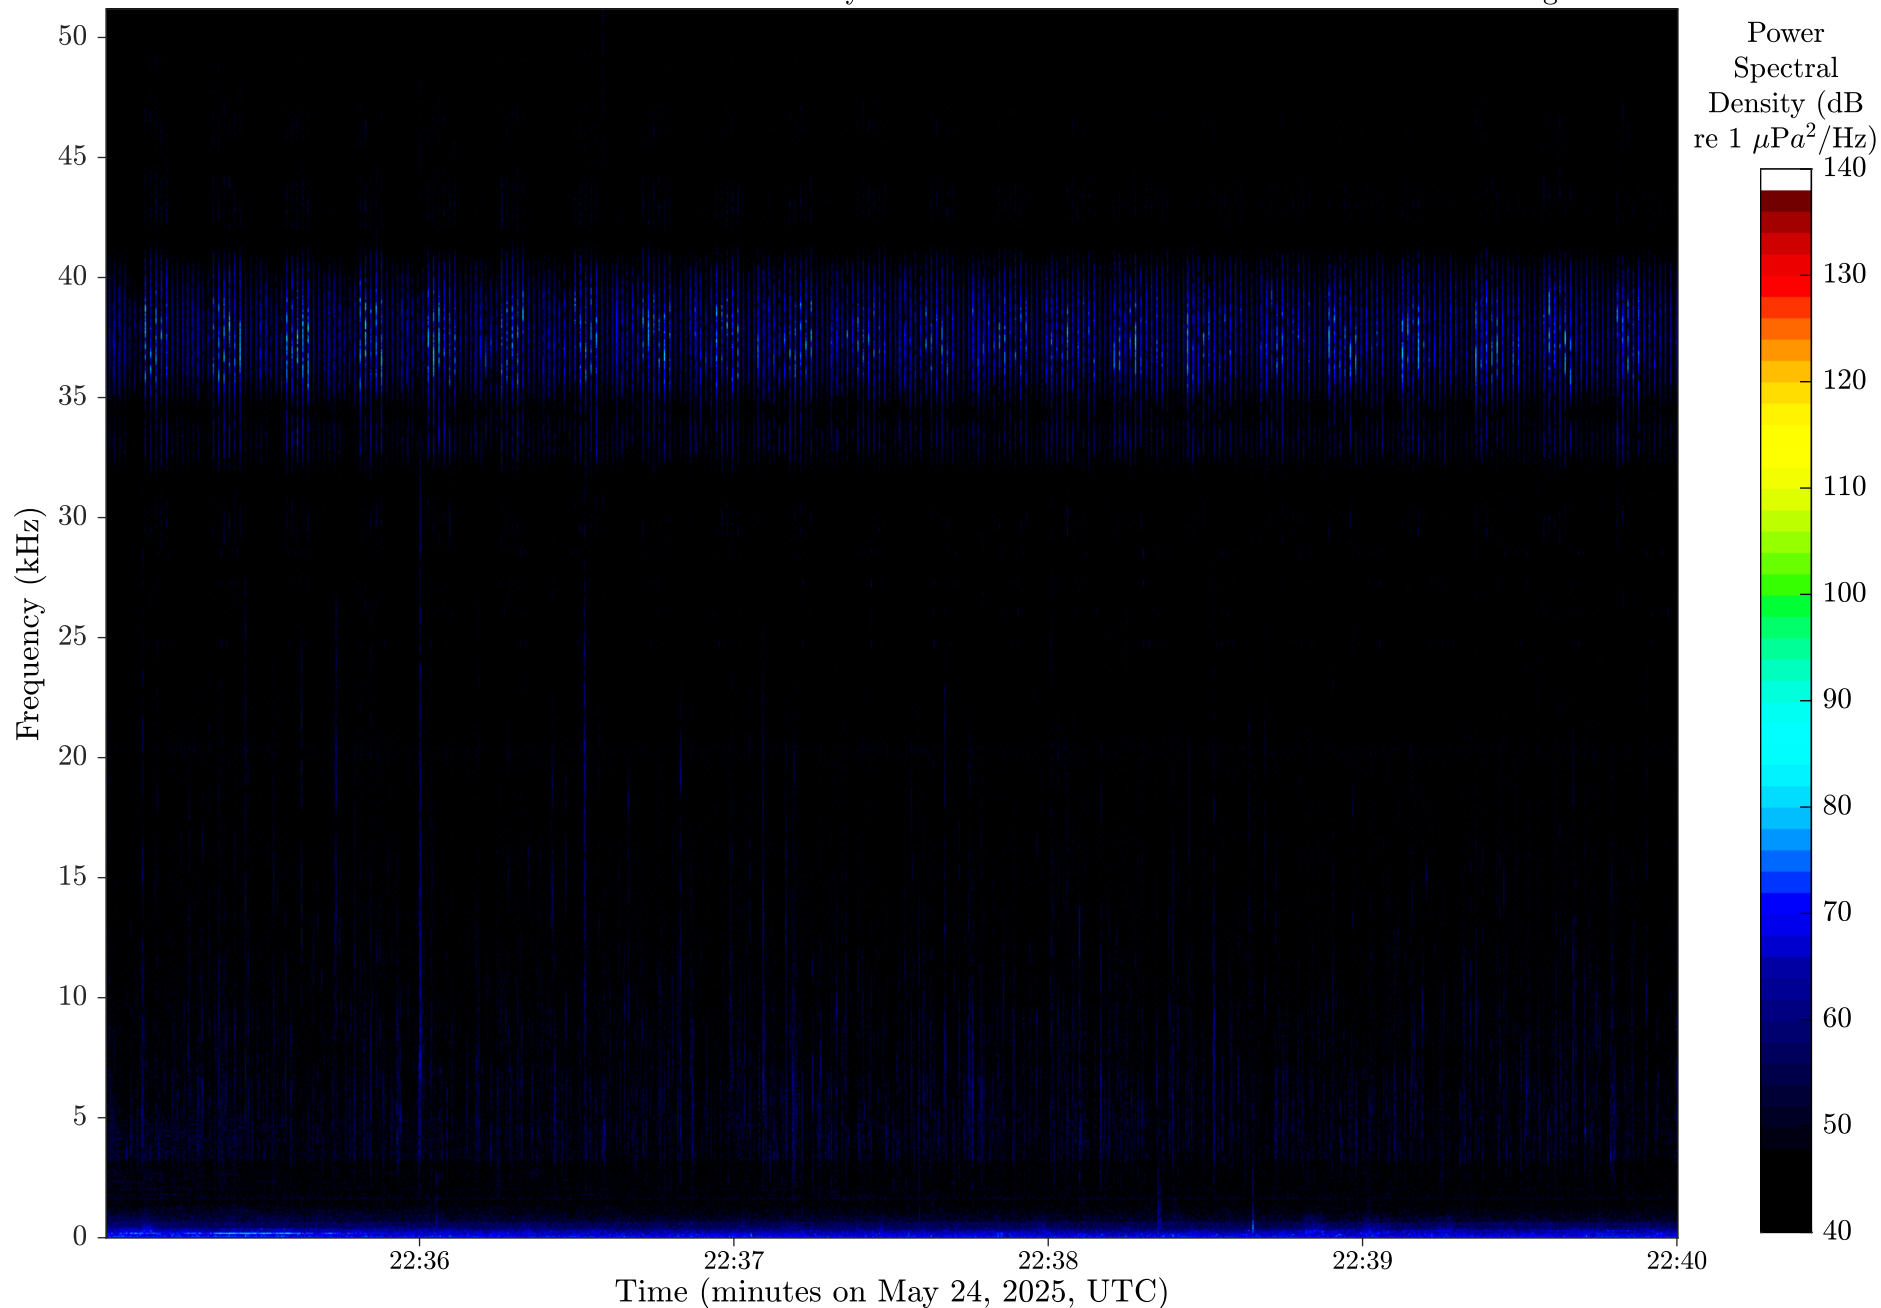


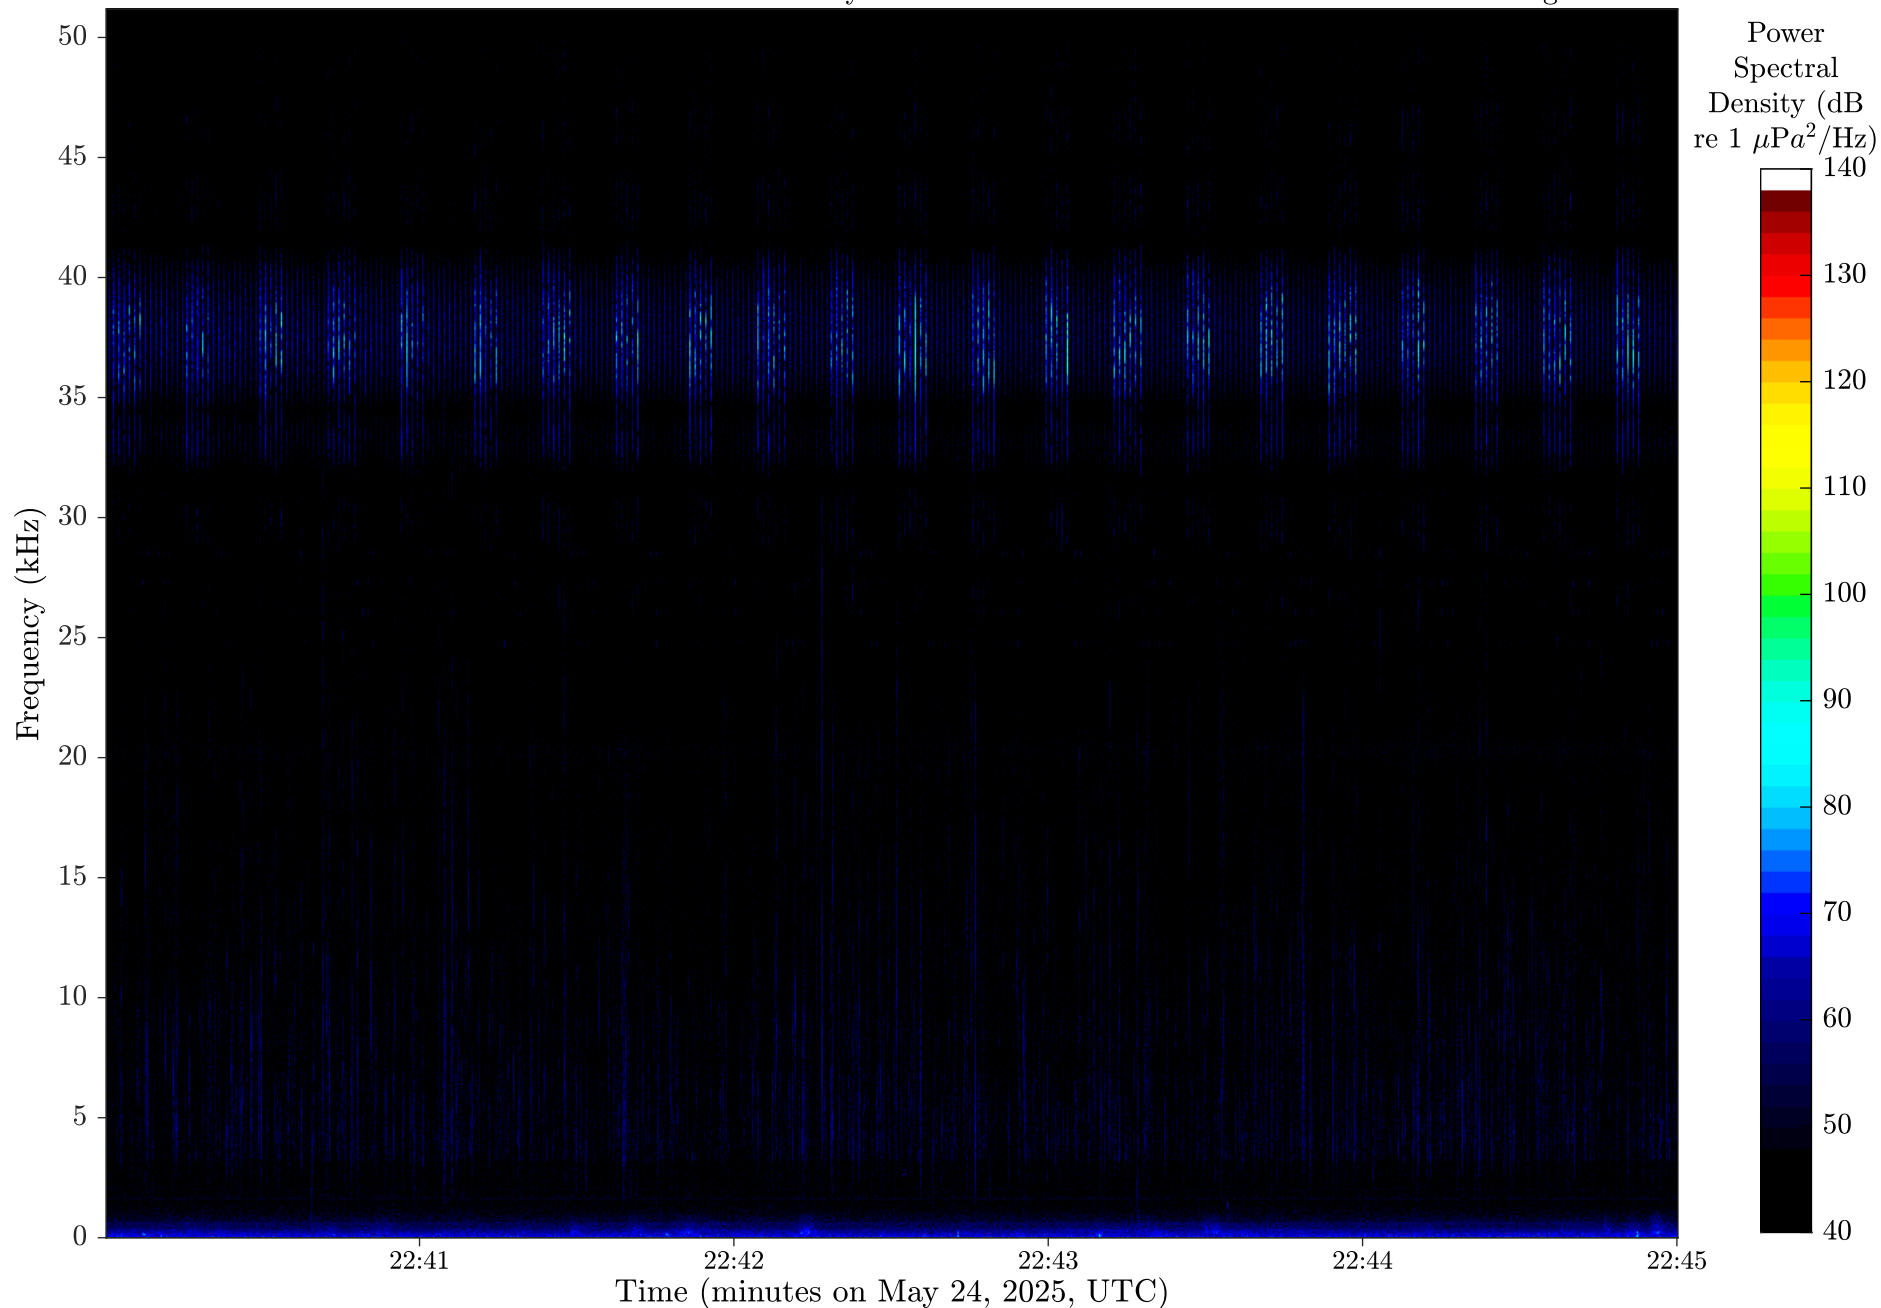

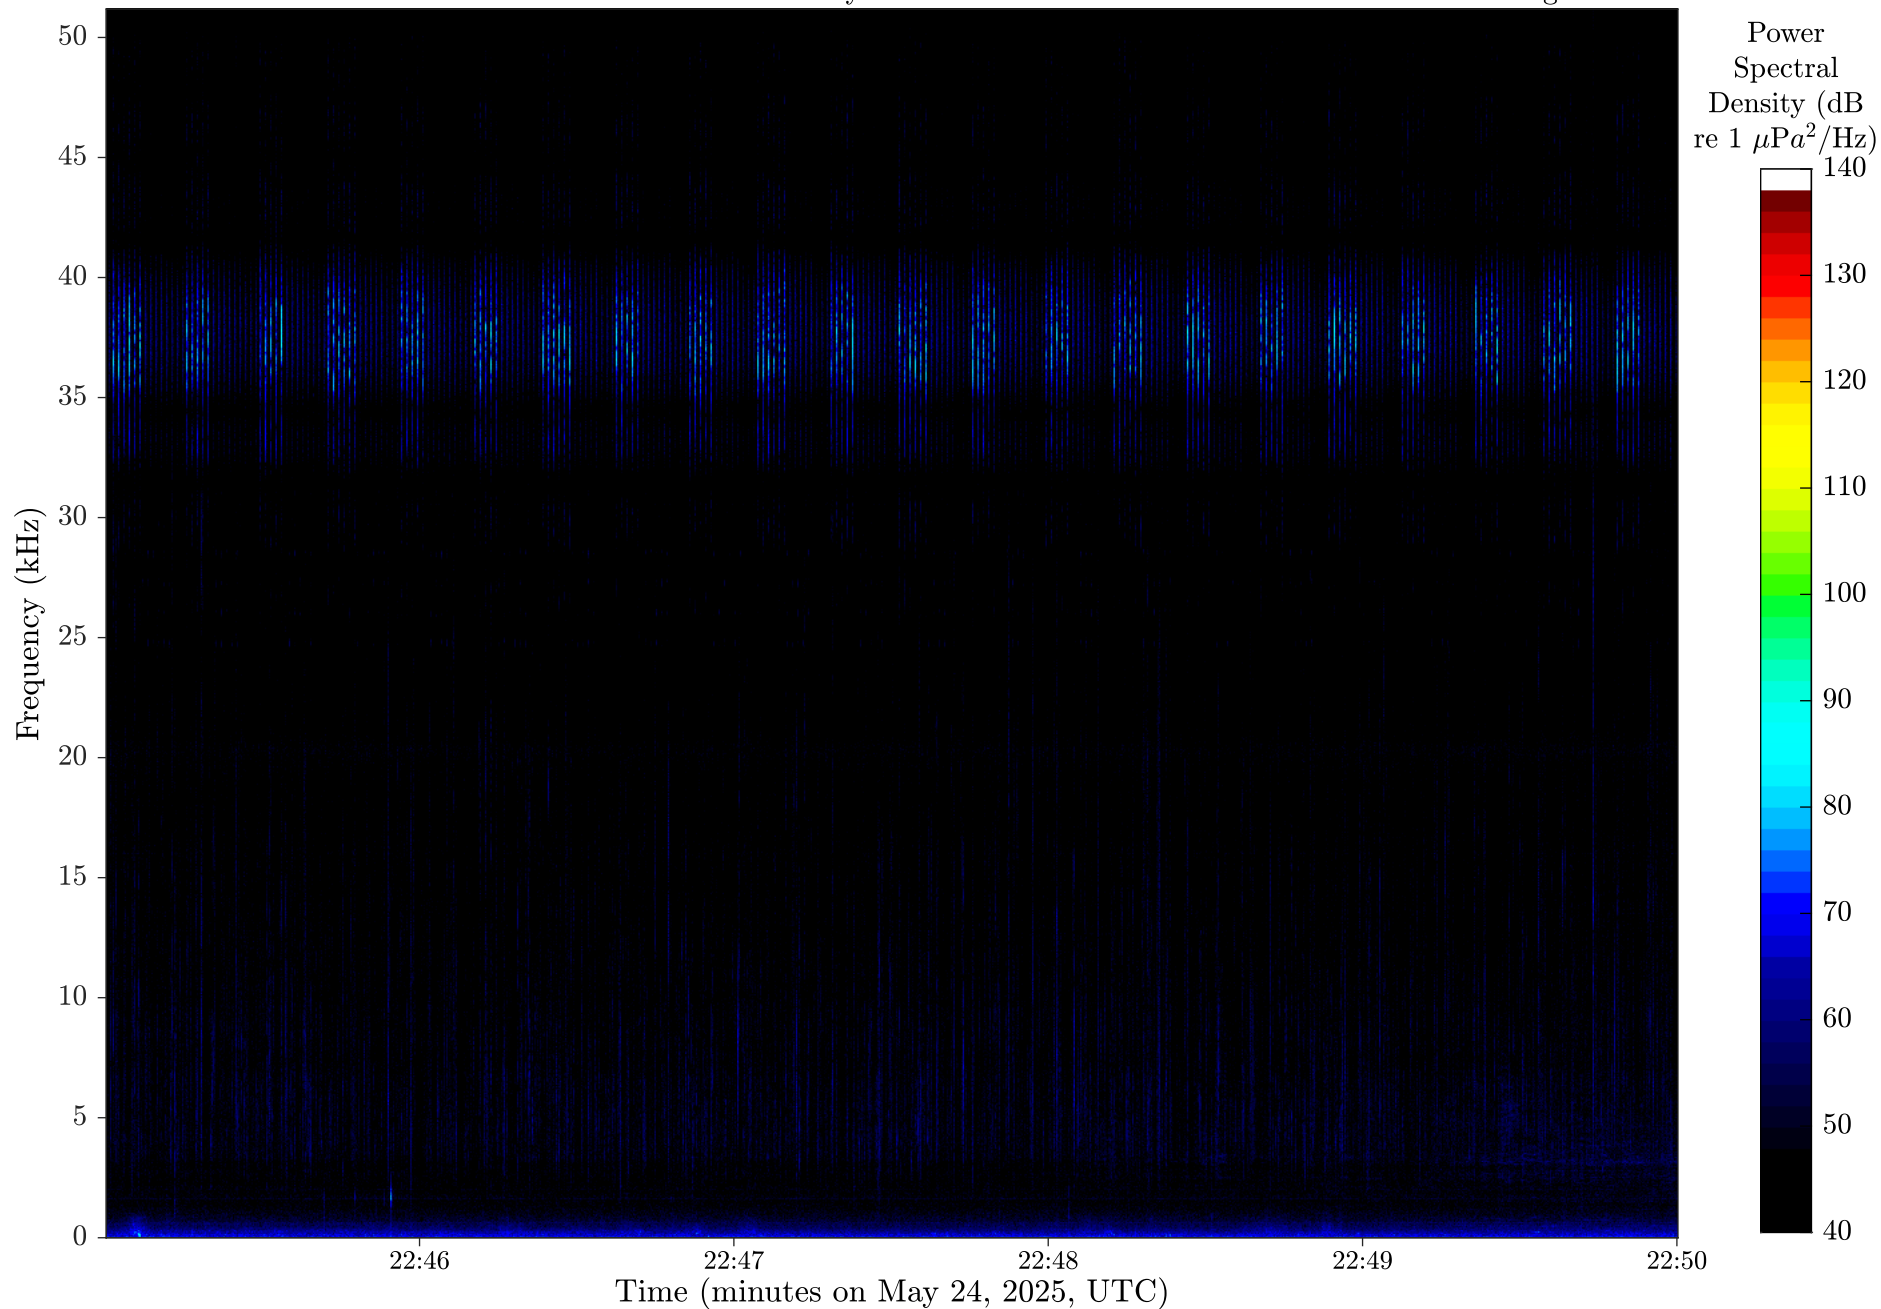


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:45:20 UTC

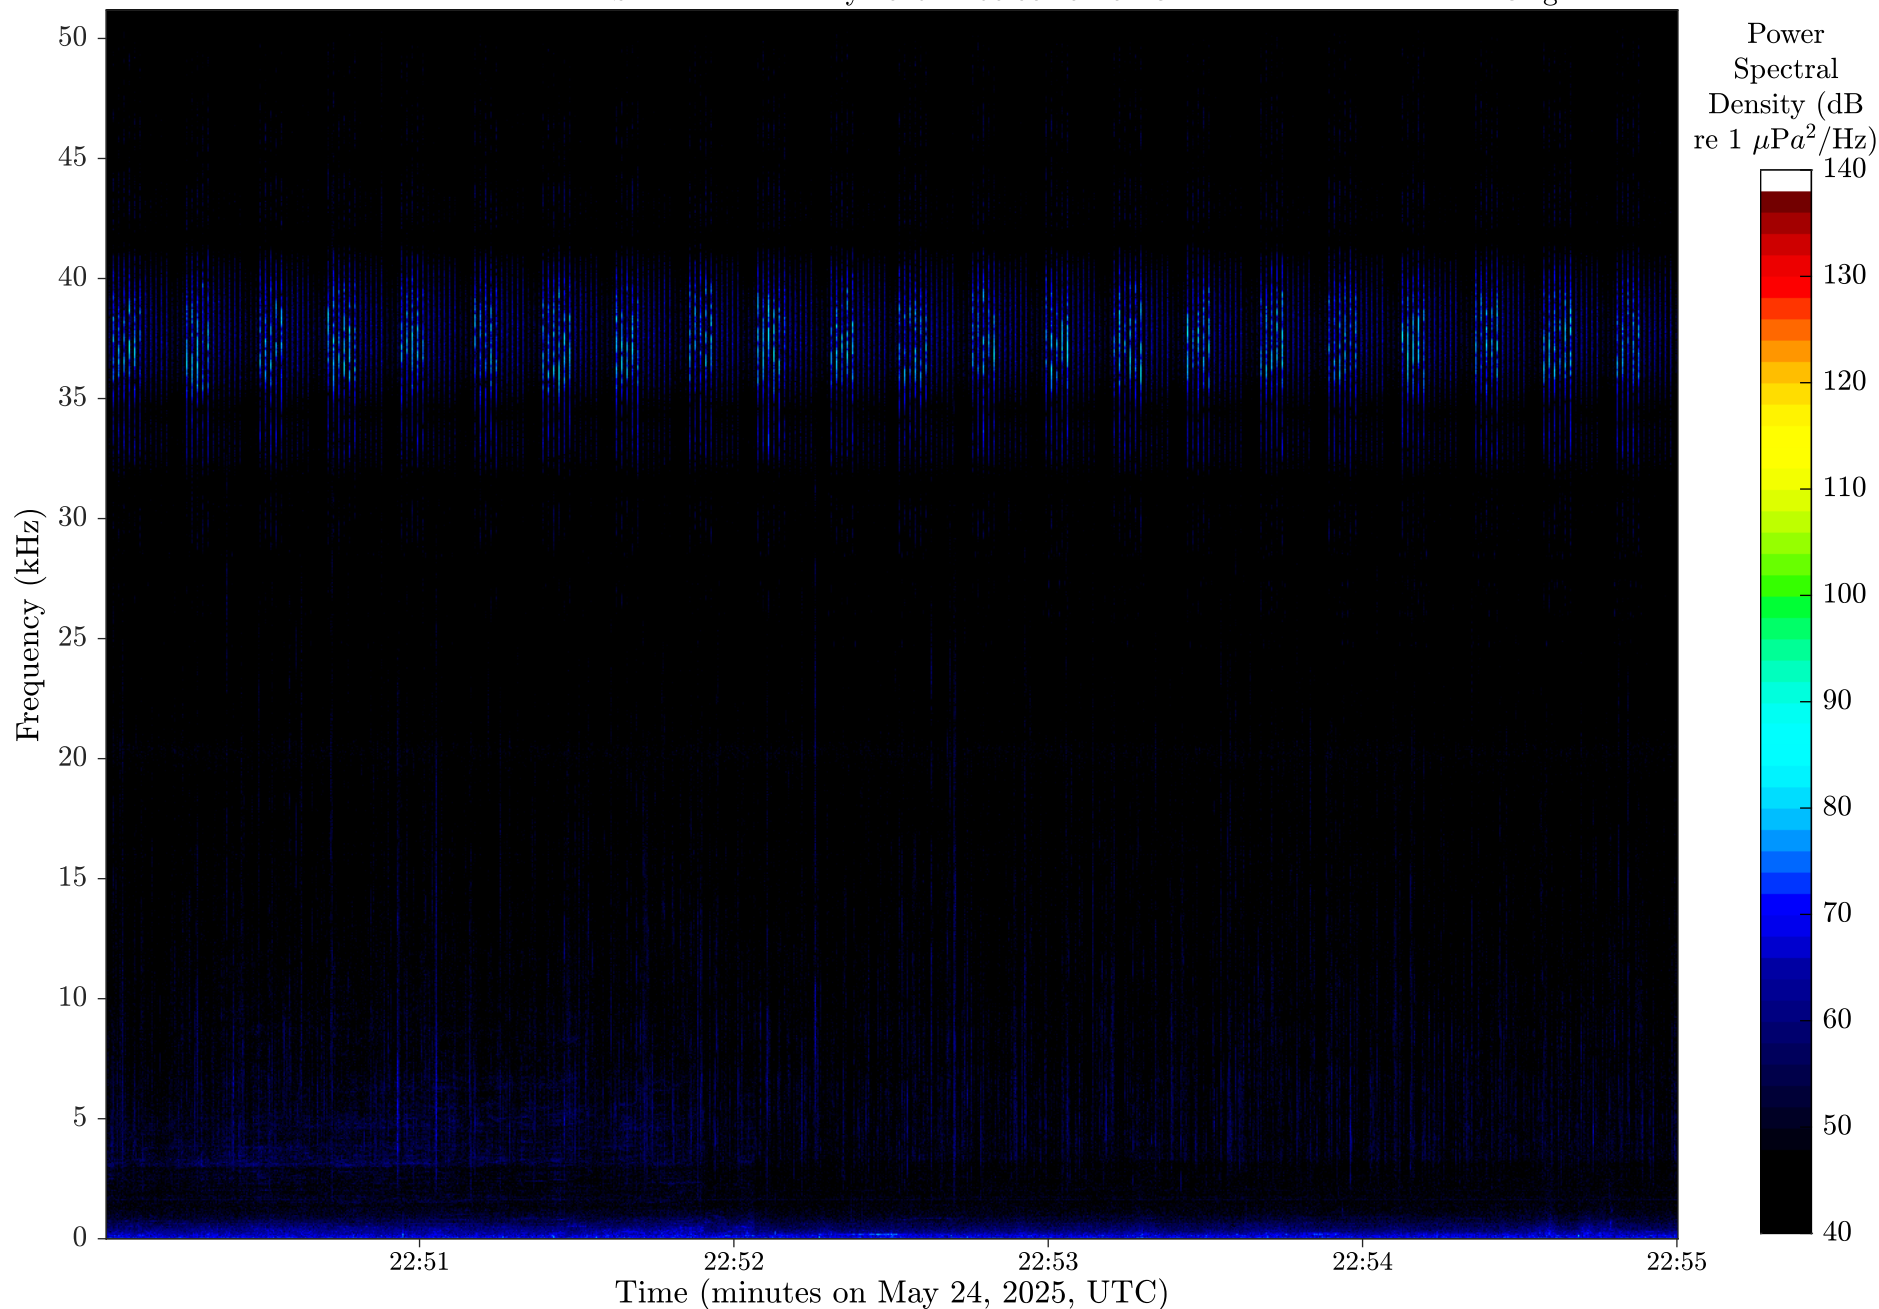


Comments: 34.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:45:27 UTC

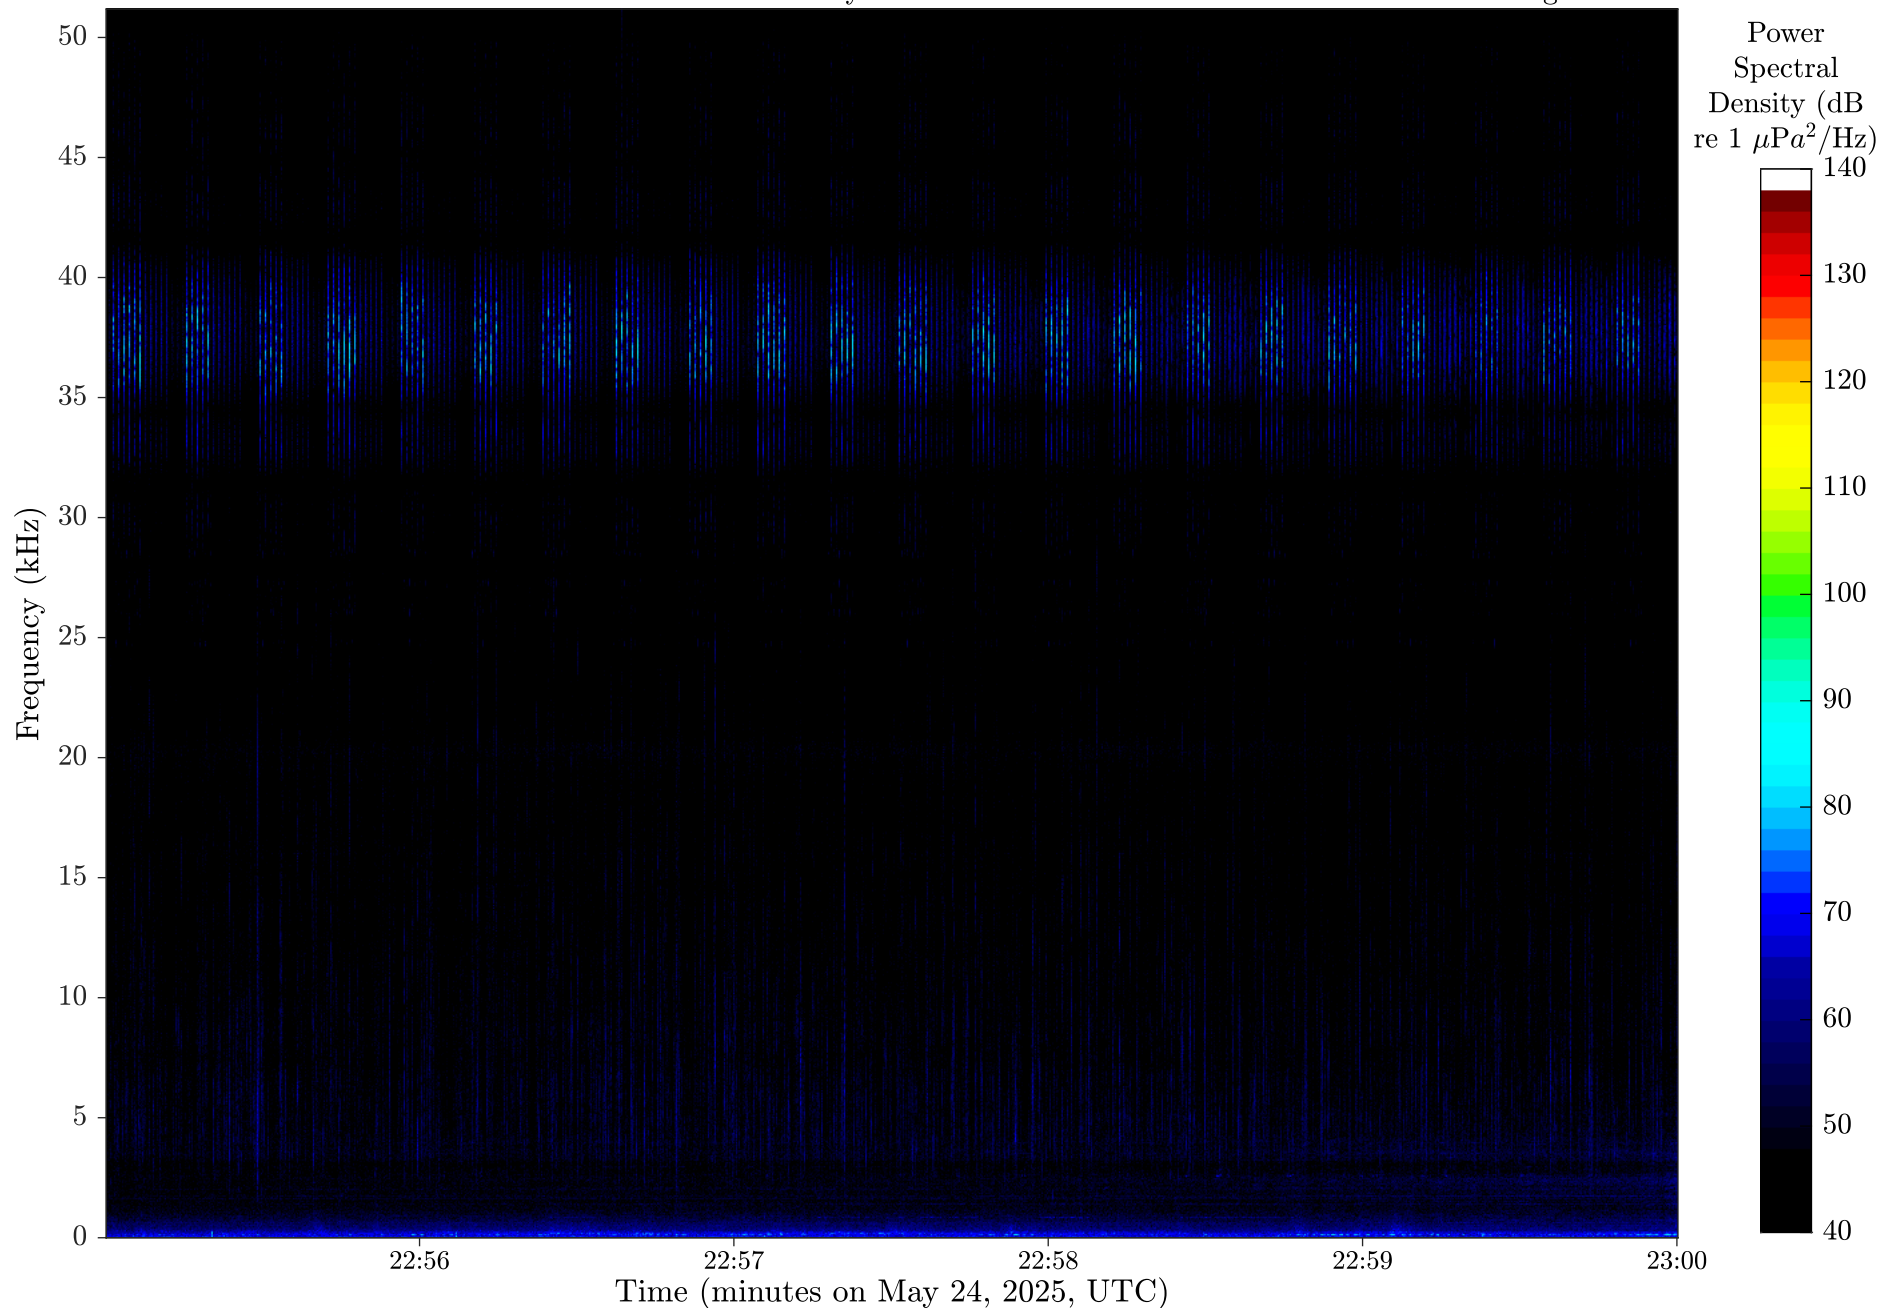

Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:45:34 UTC

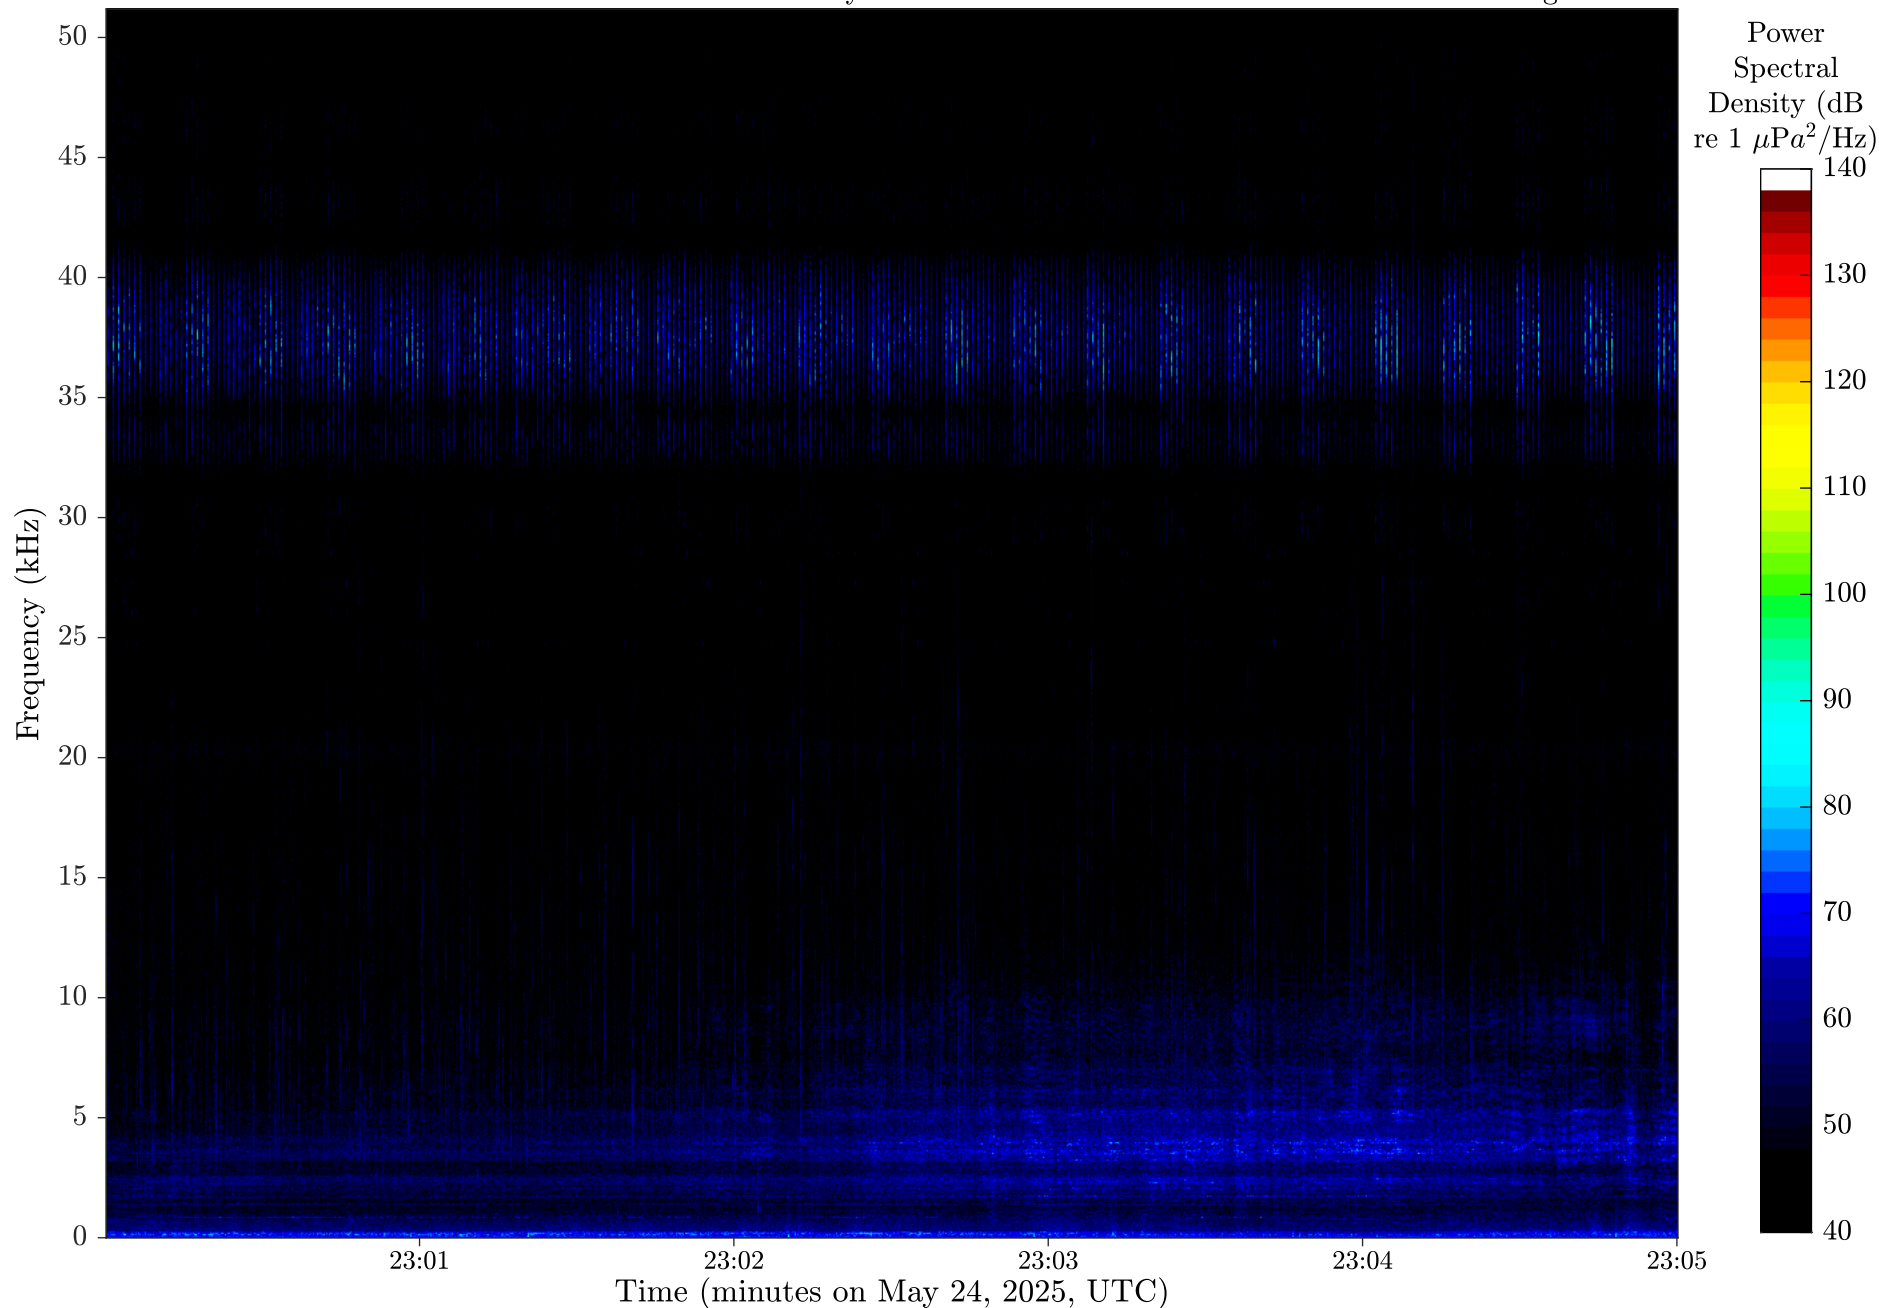

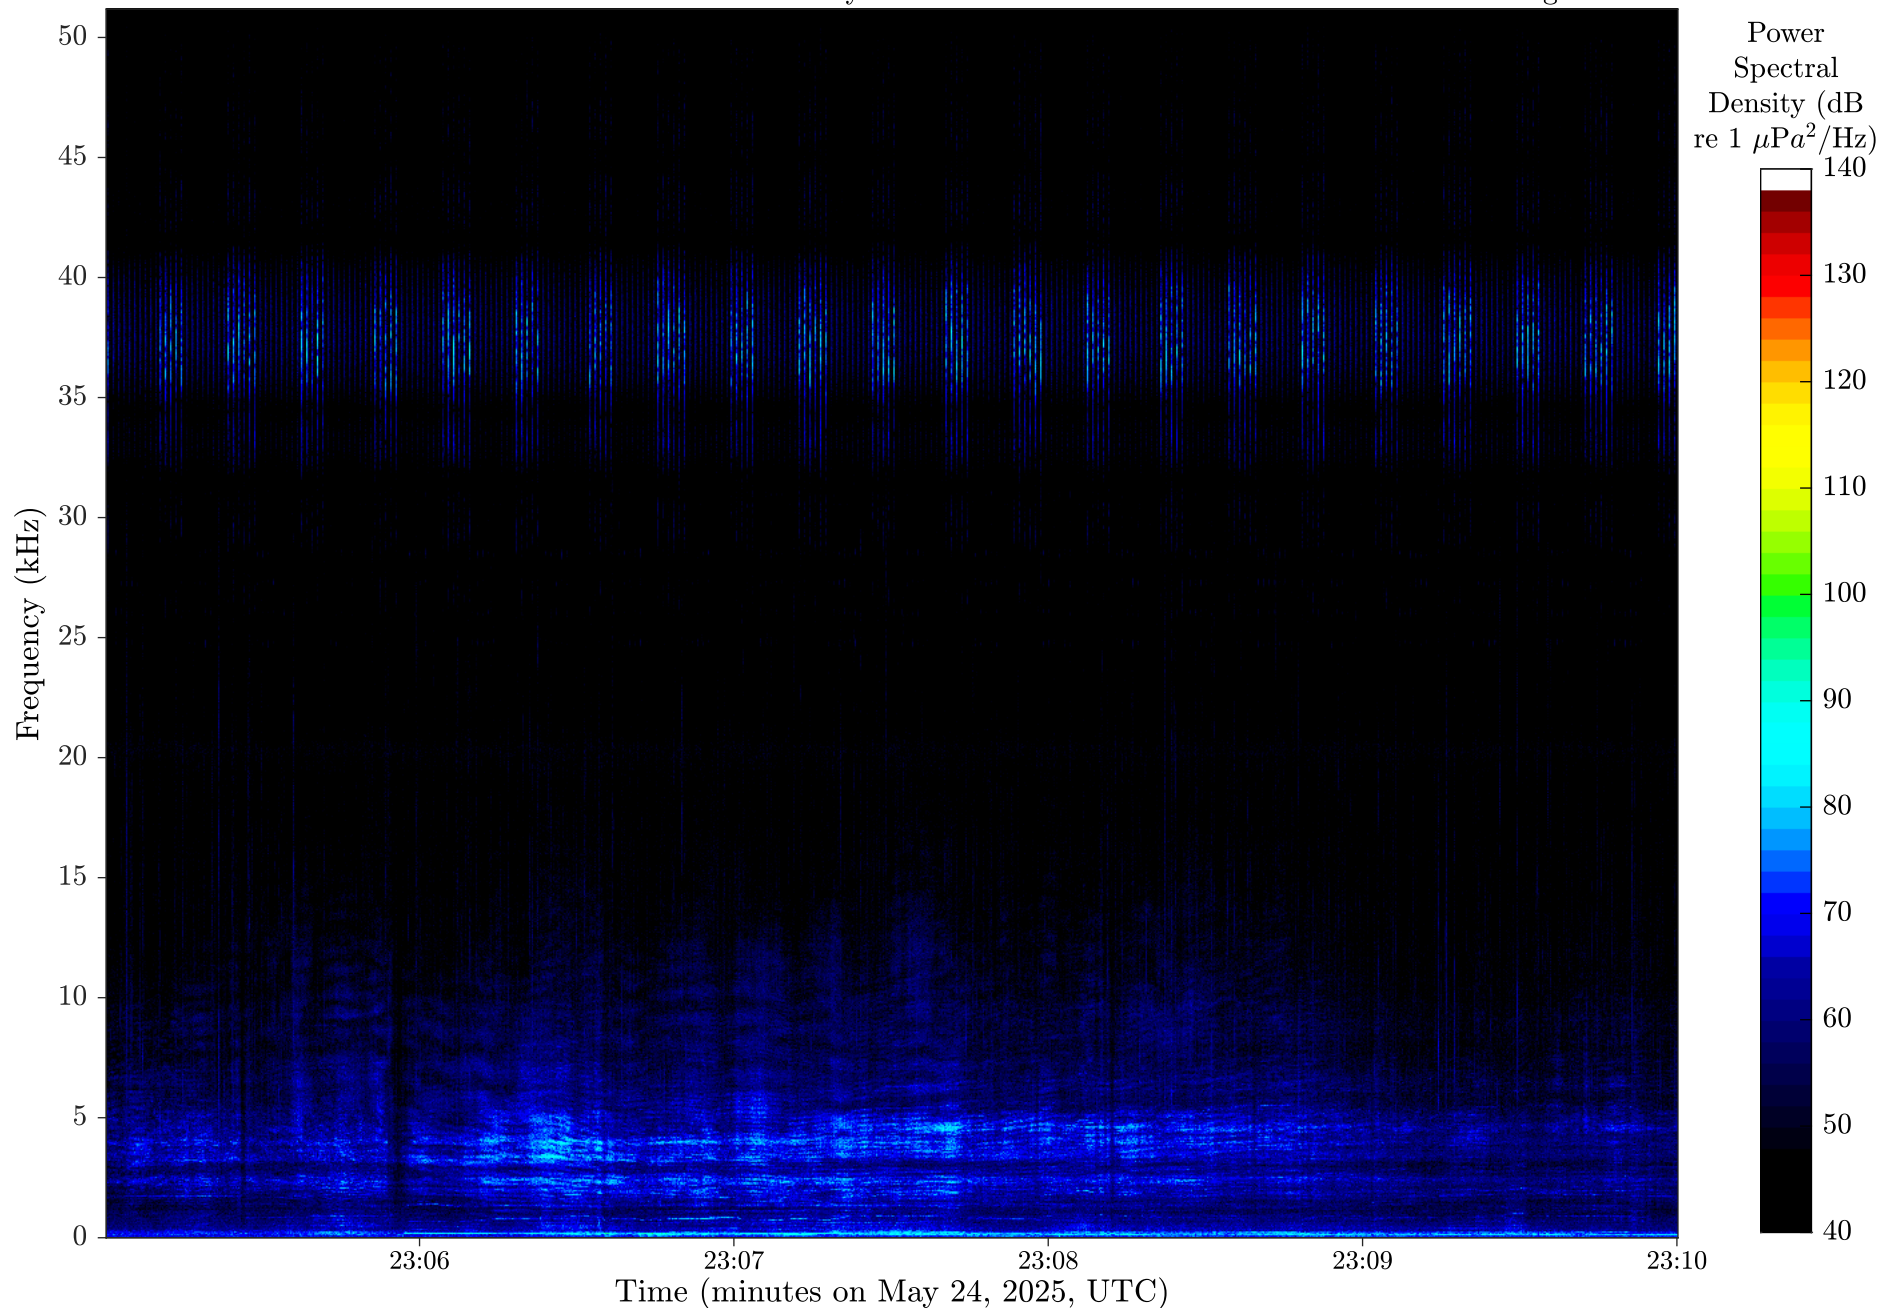


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:45:48 UTC

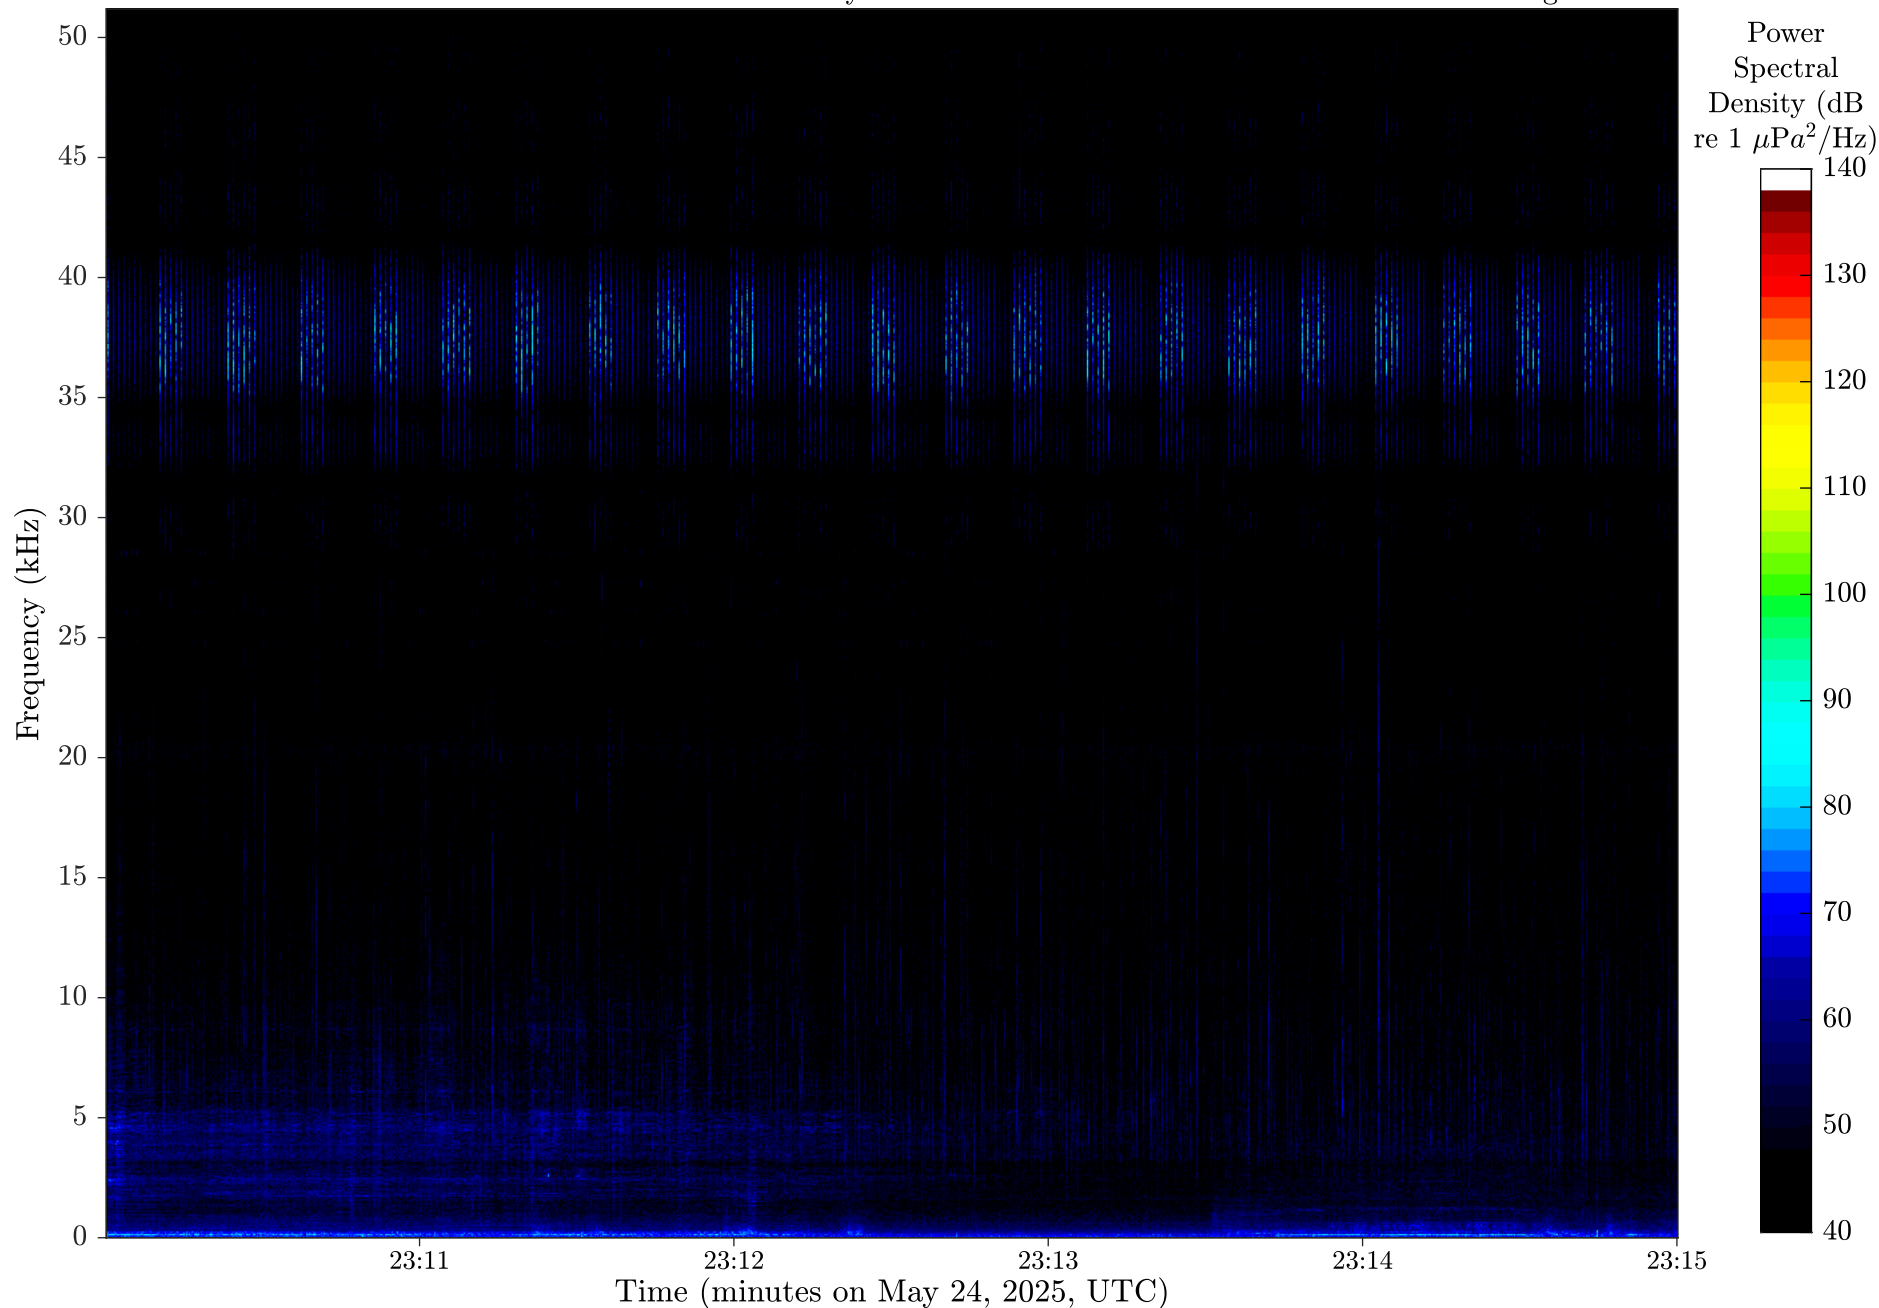


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:45:55 UTC

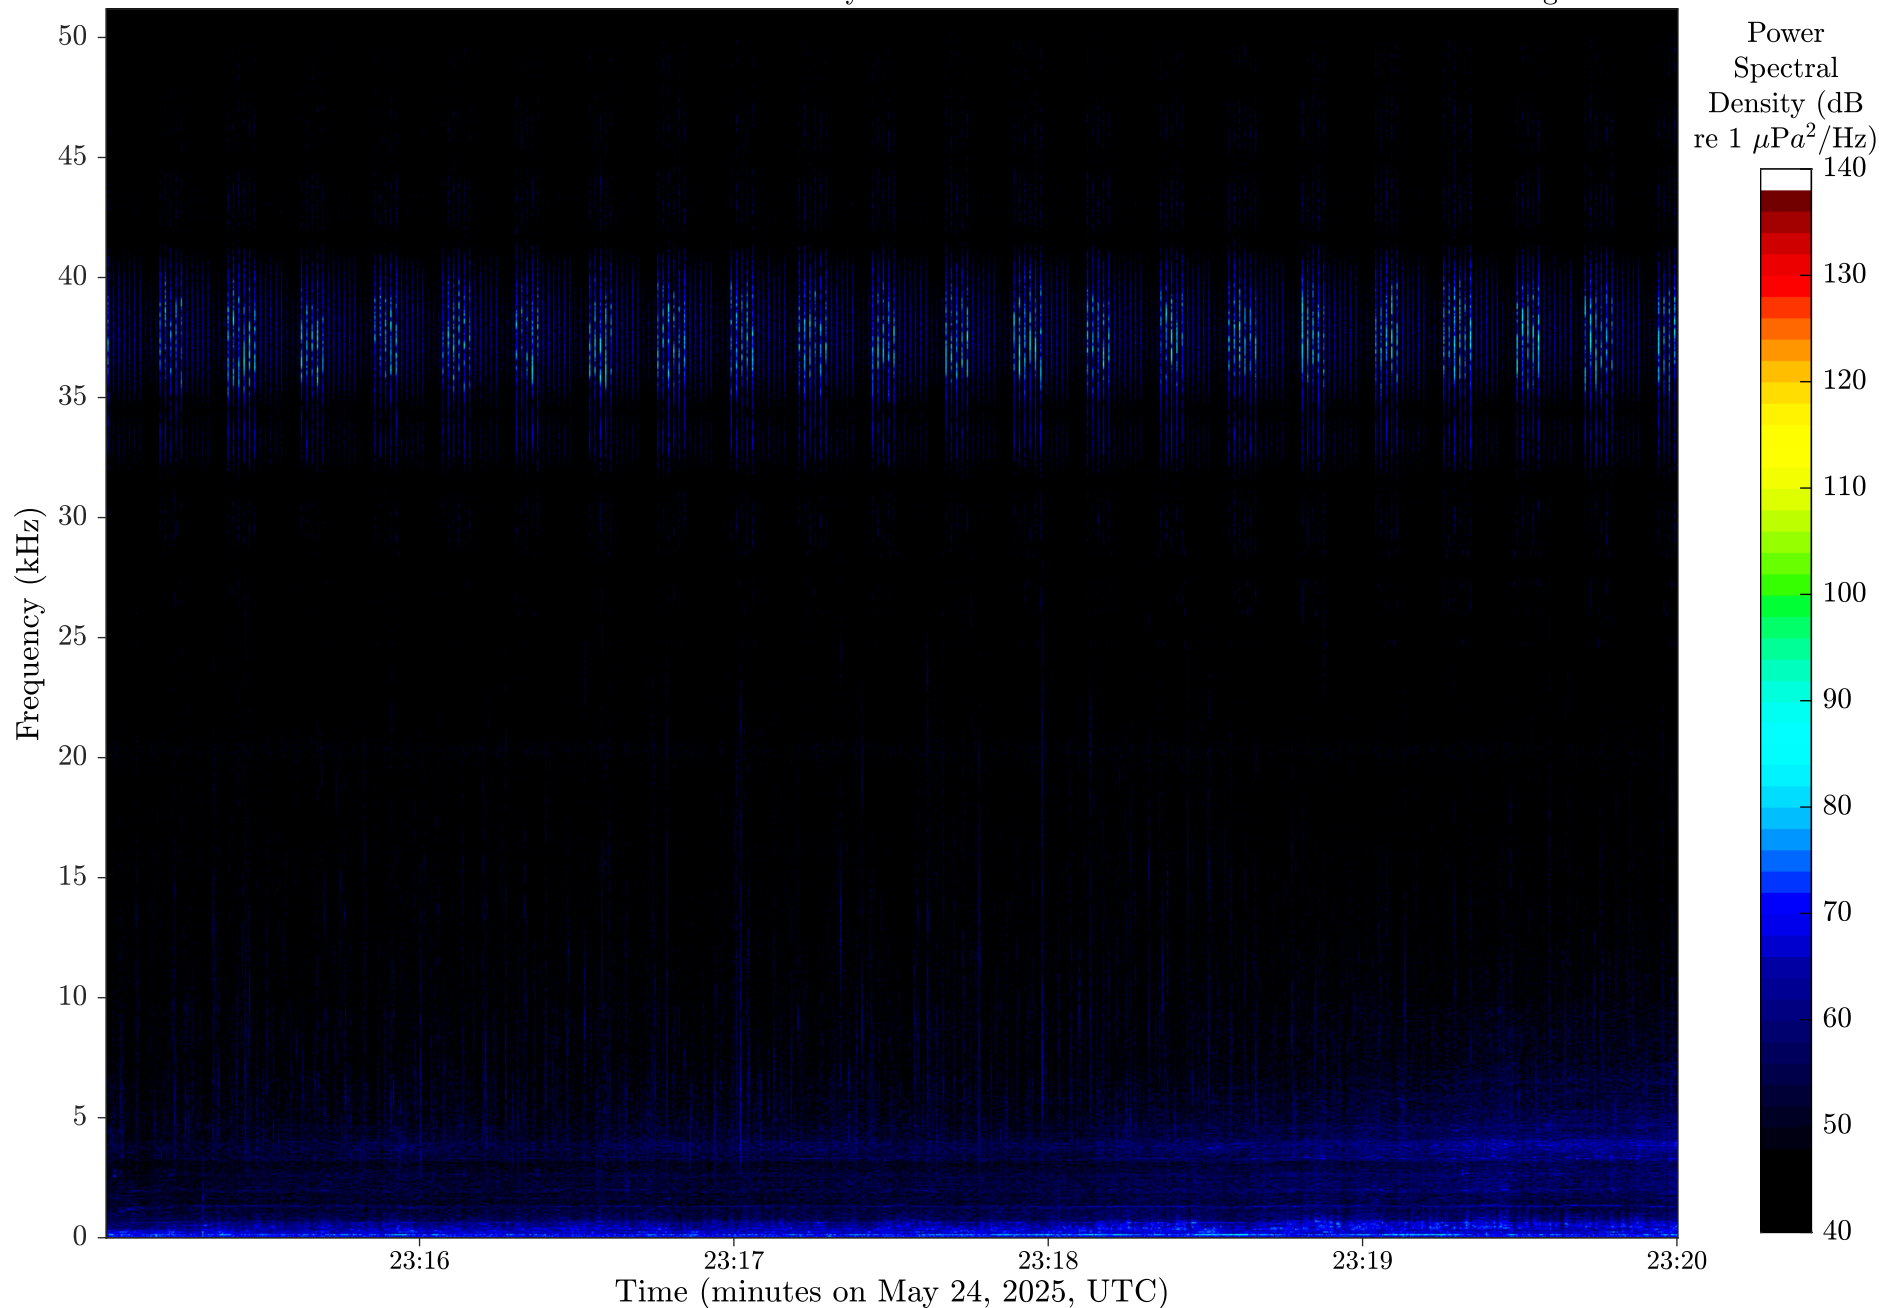


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:03 UTC

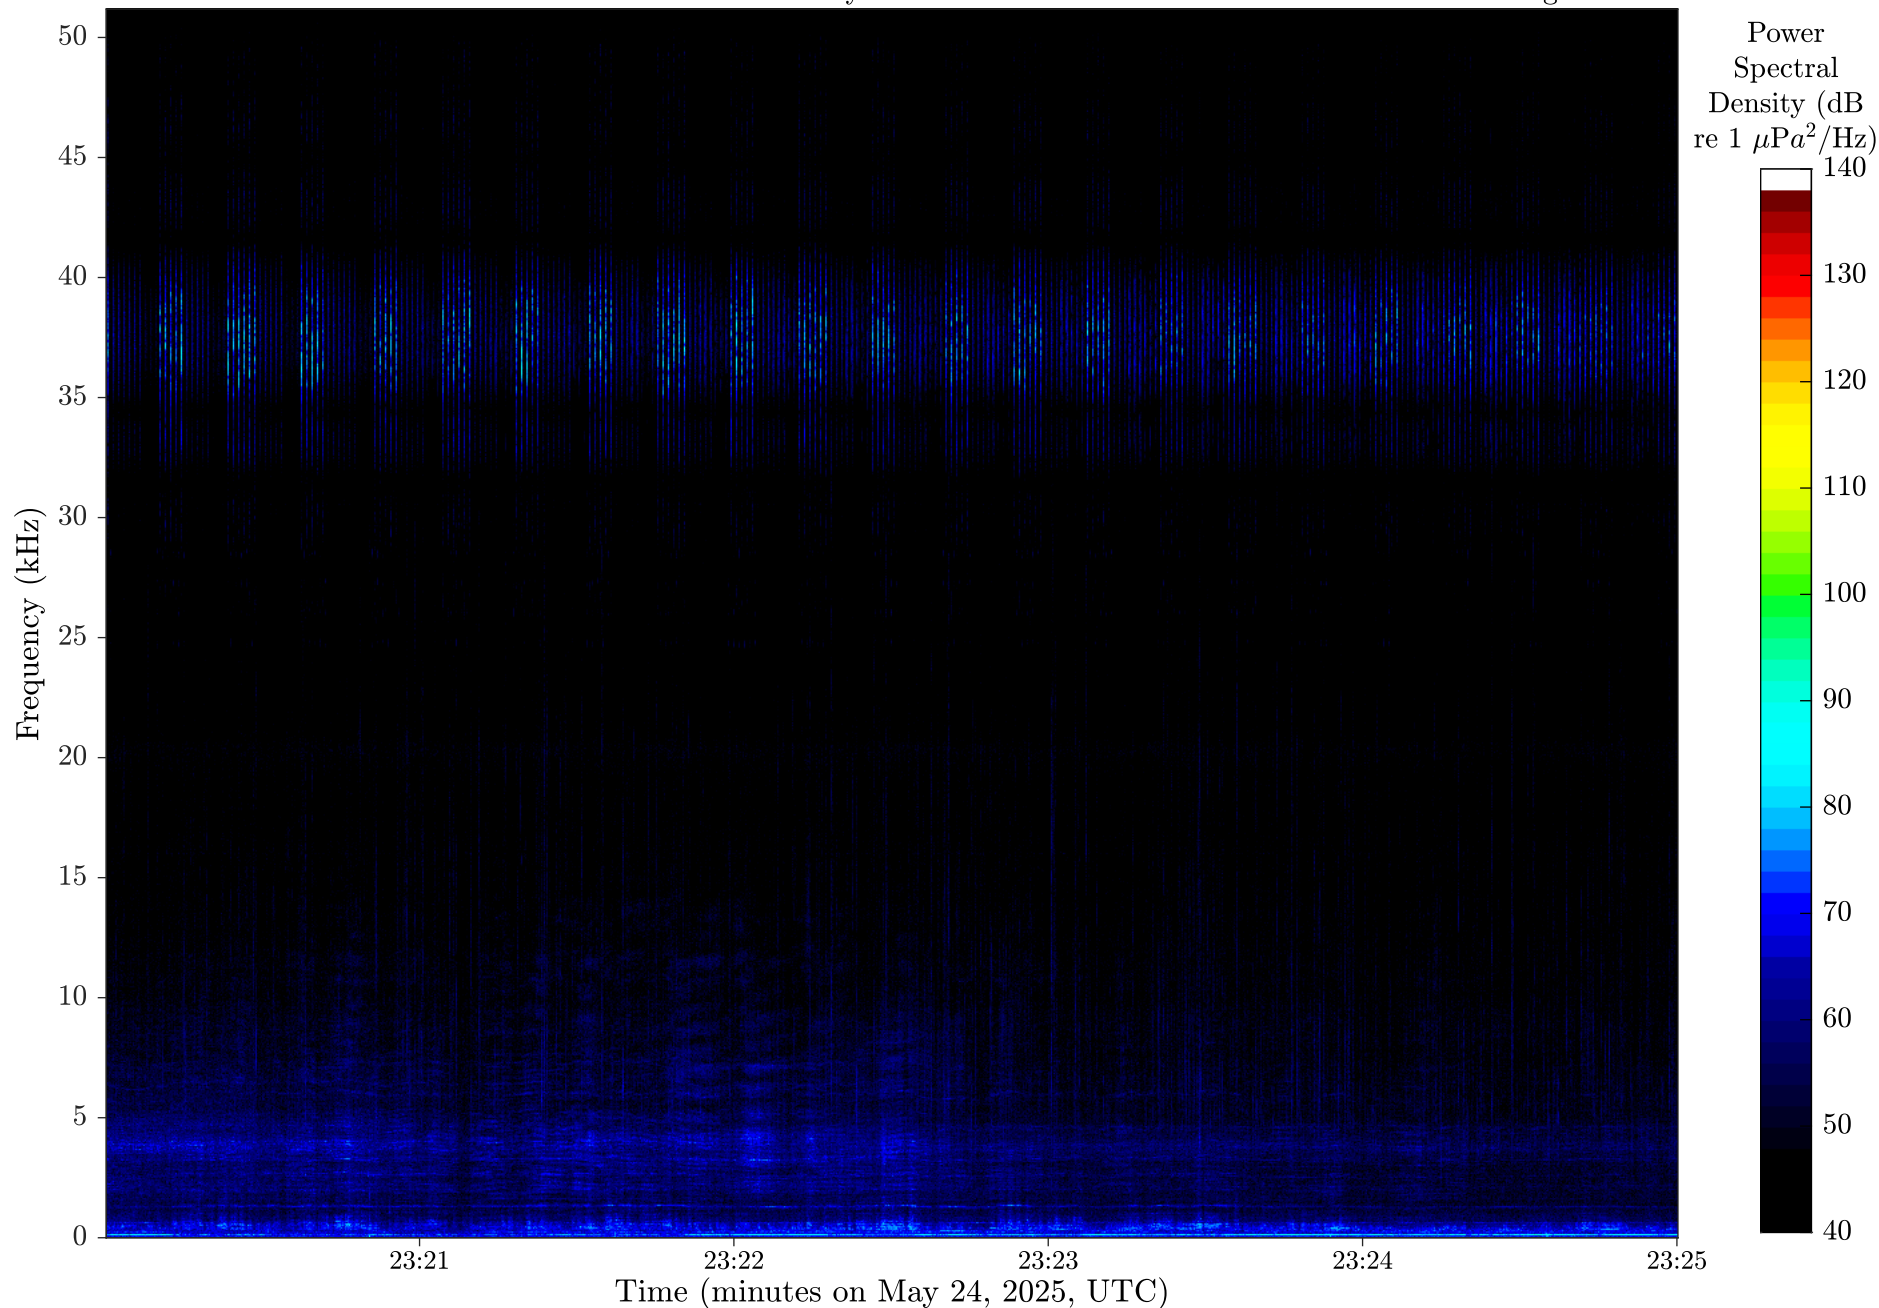


Comments: 30.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:46:10 UTC

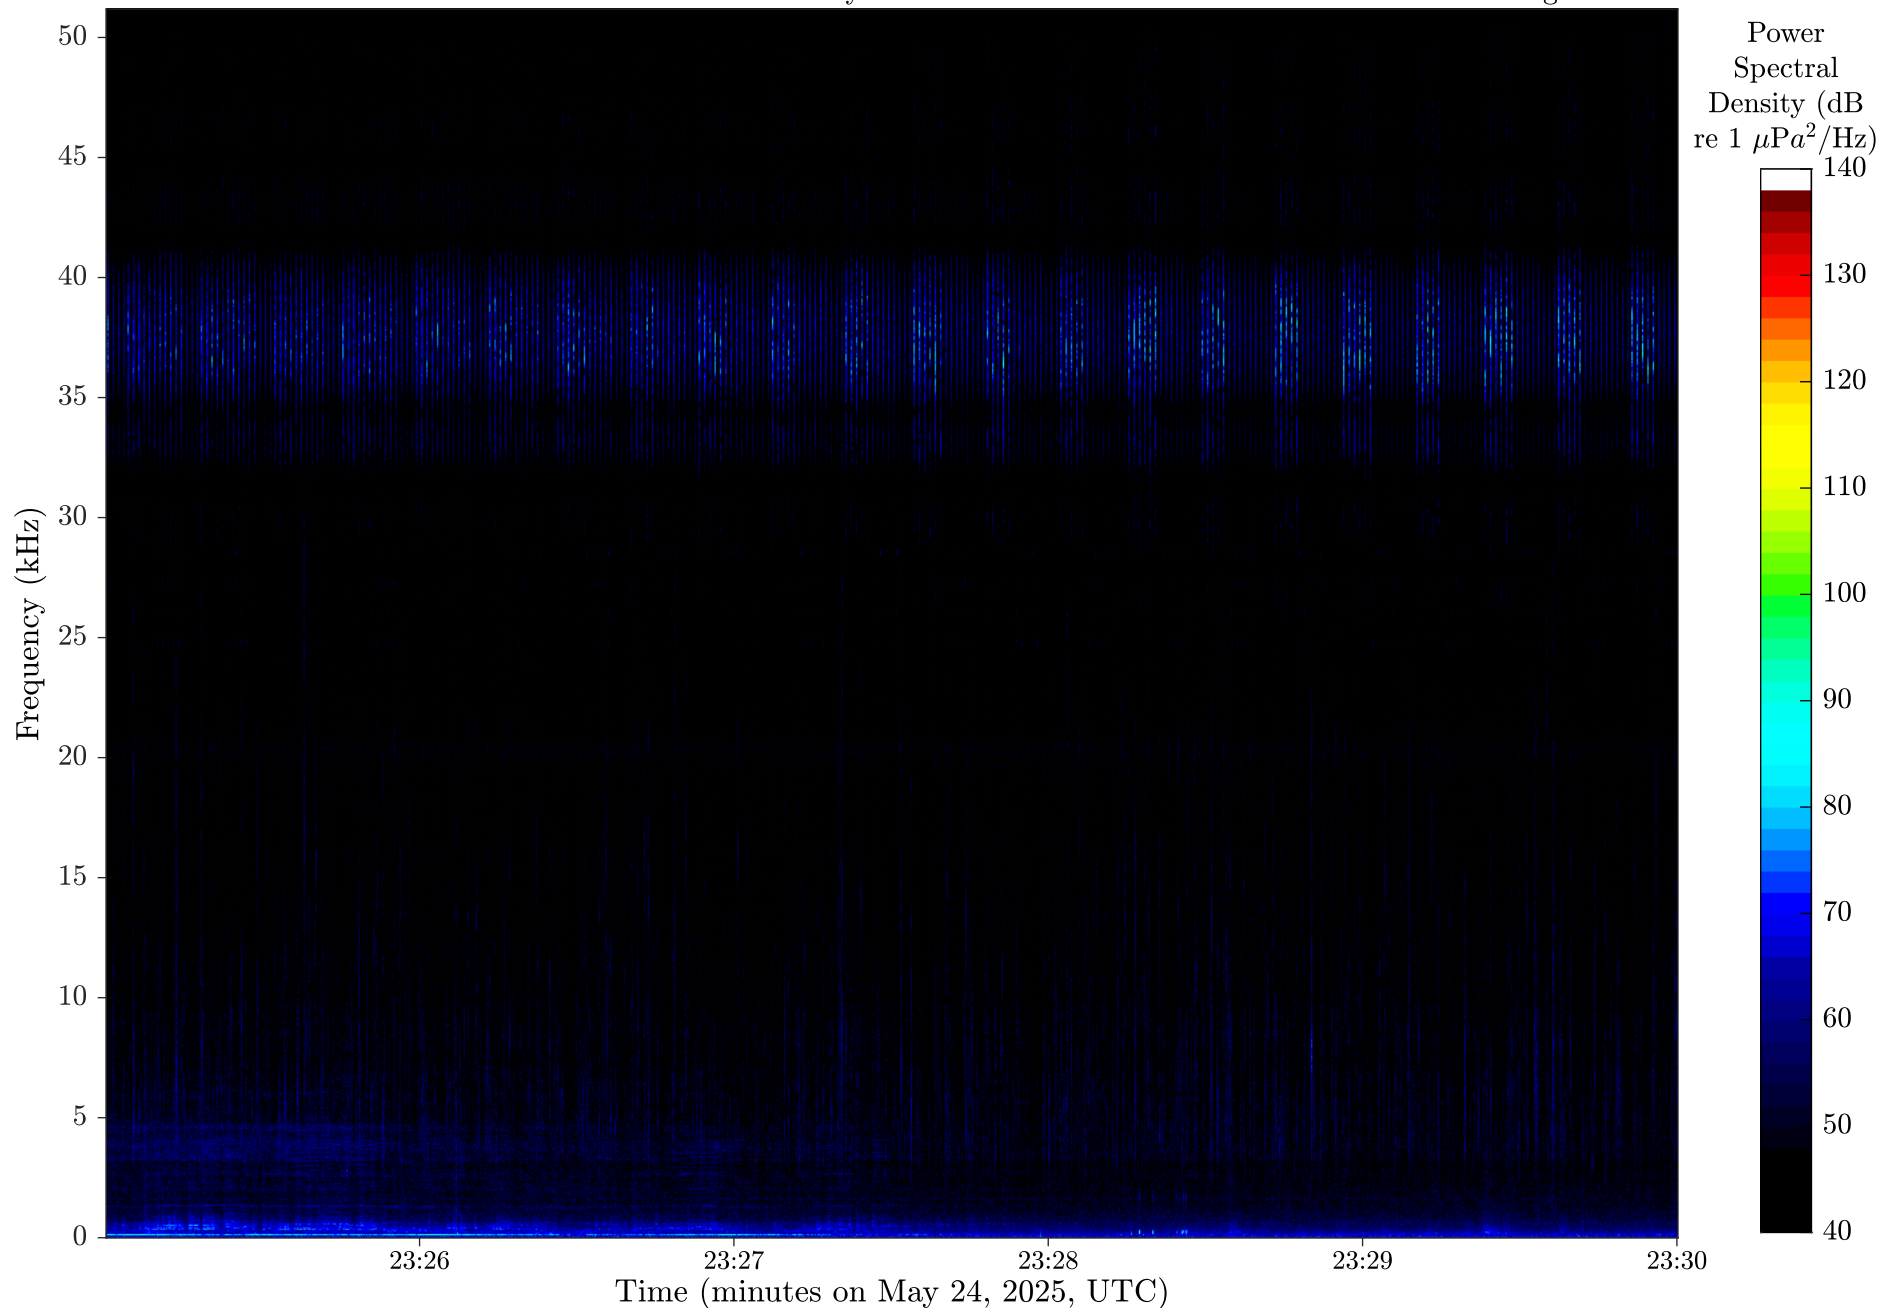

Comments: 31.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:46:18 UTC

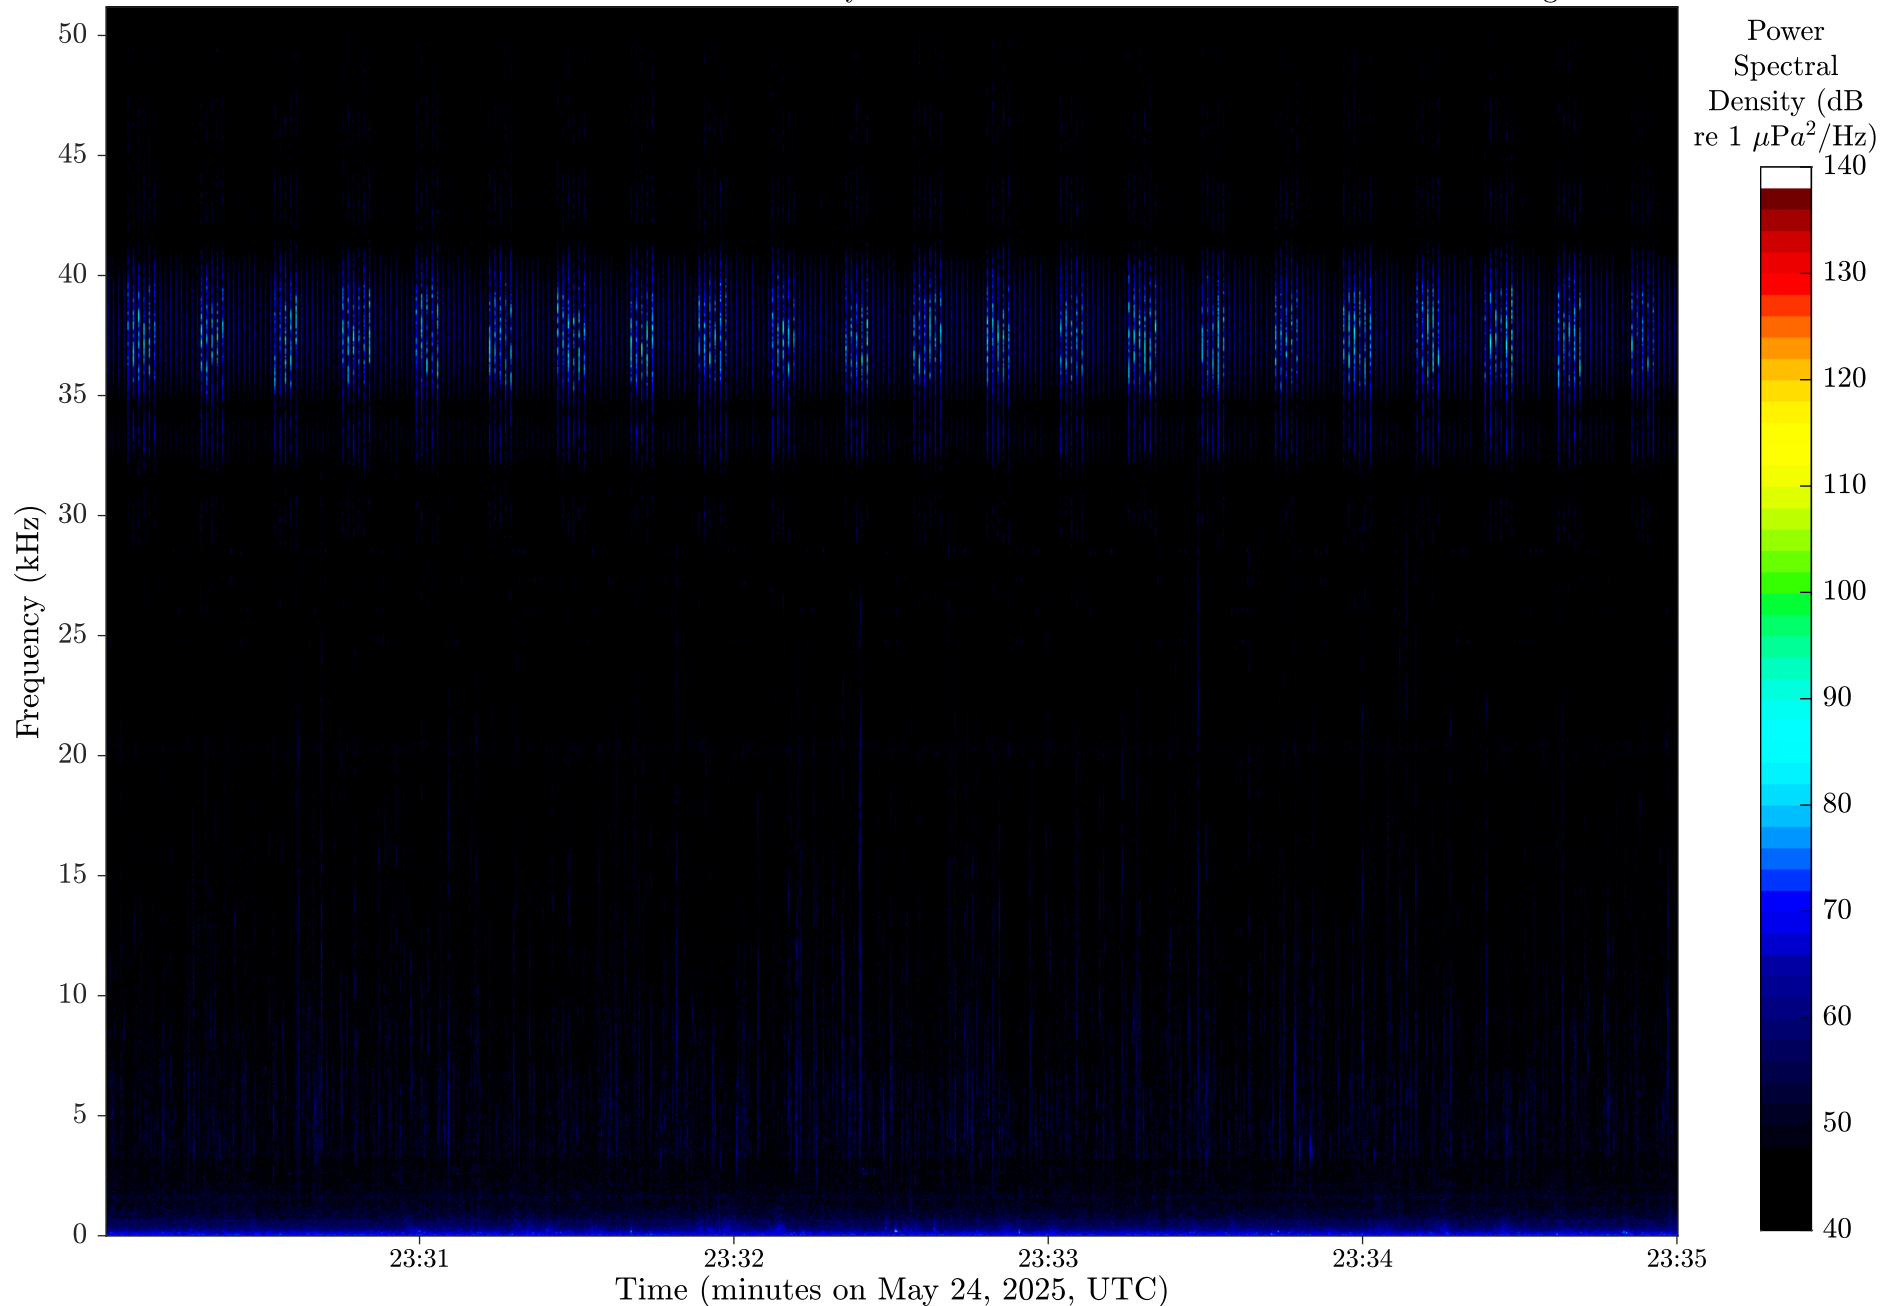

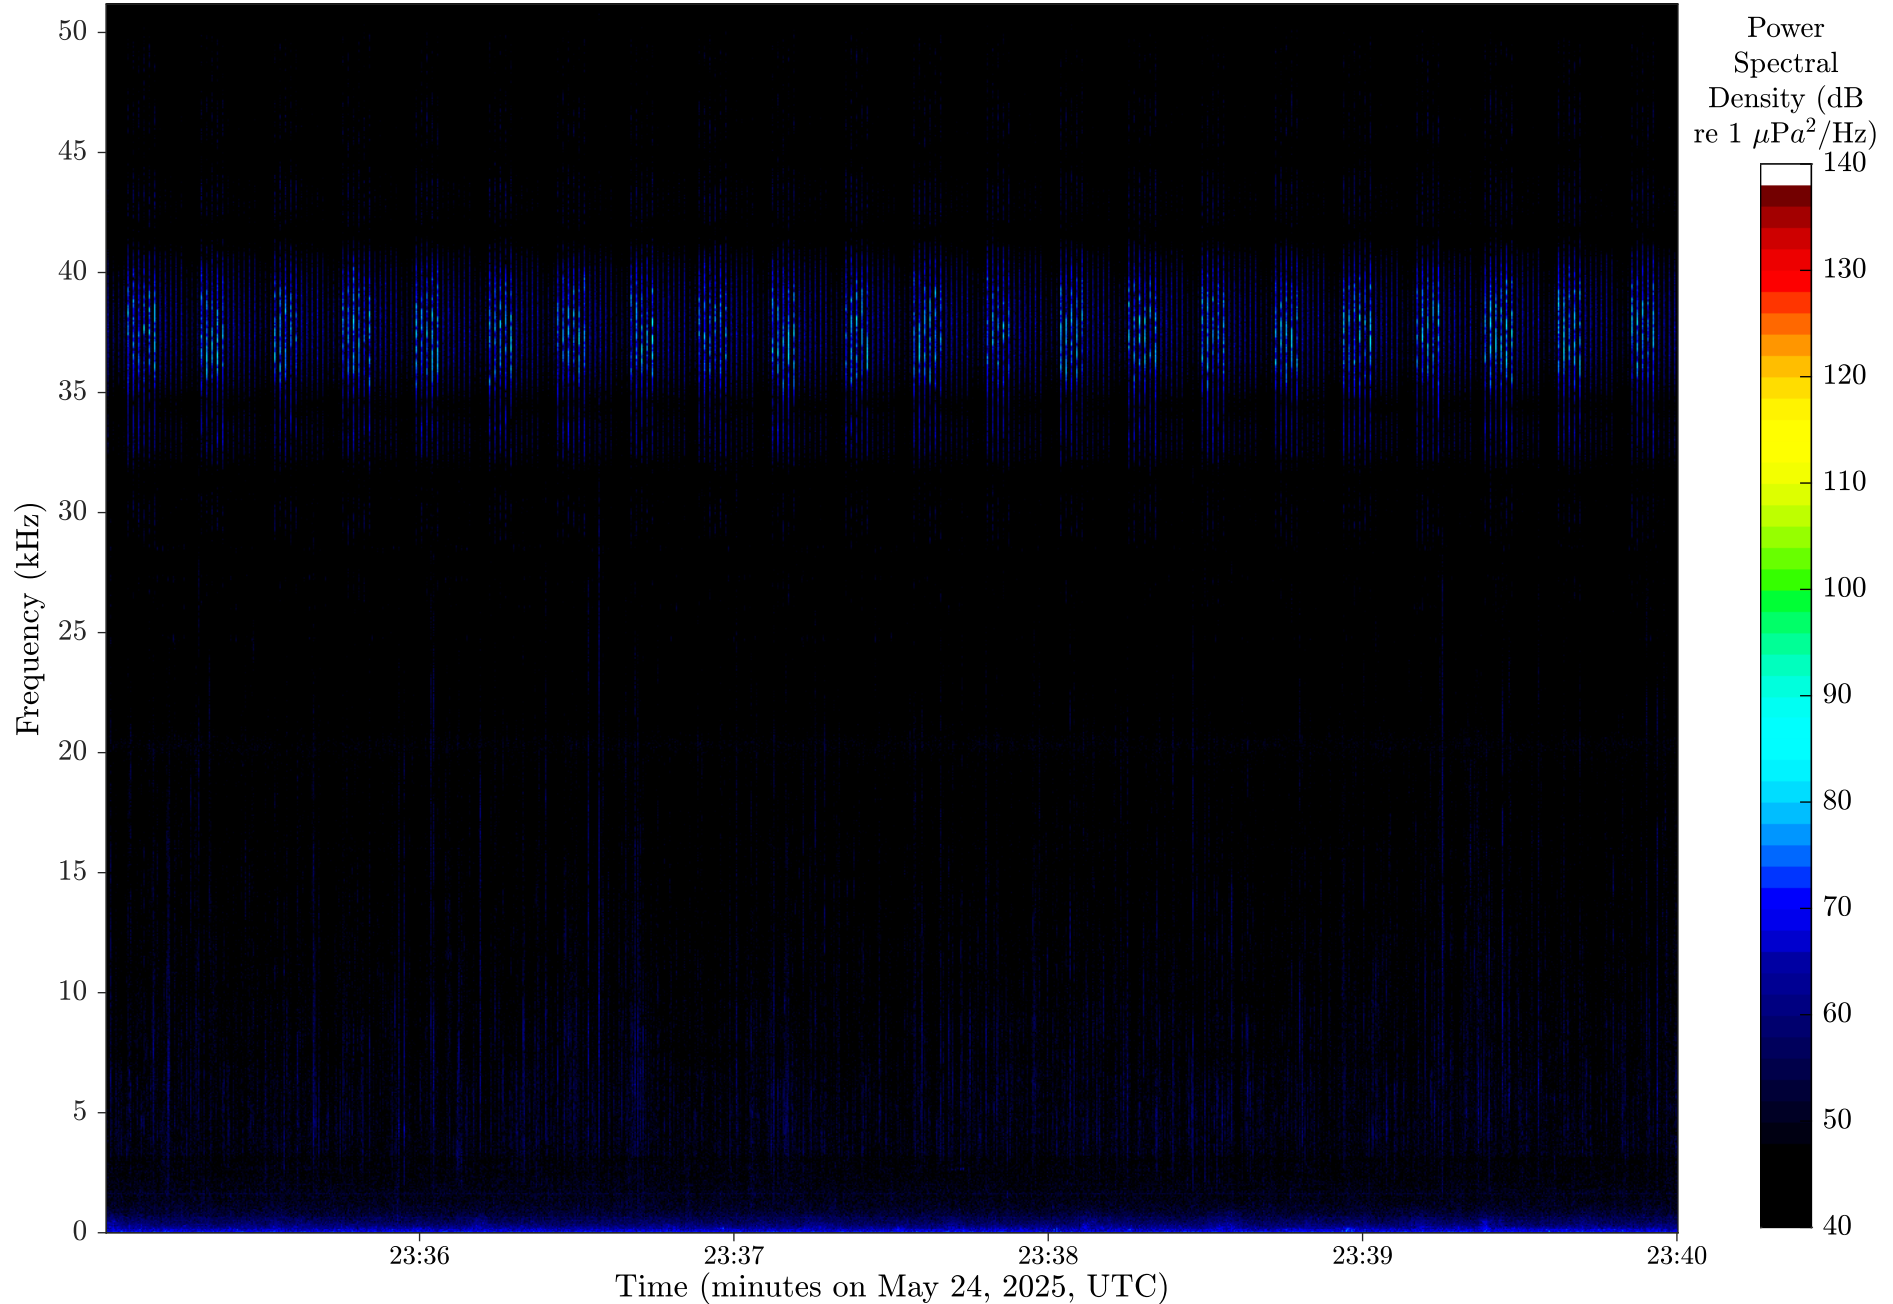


Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:33 UTC

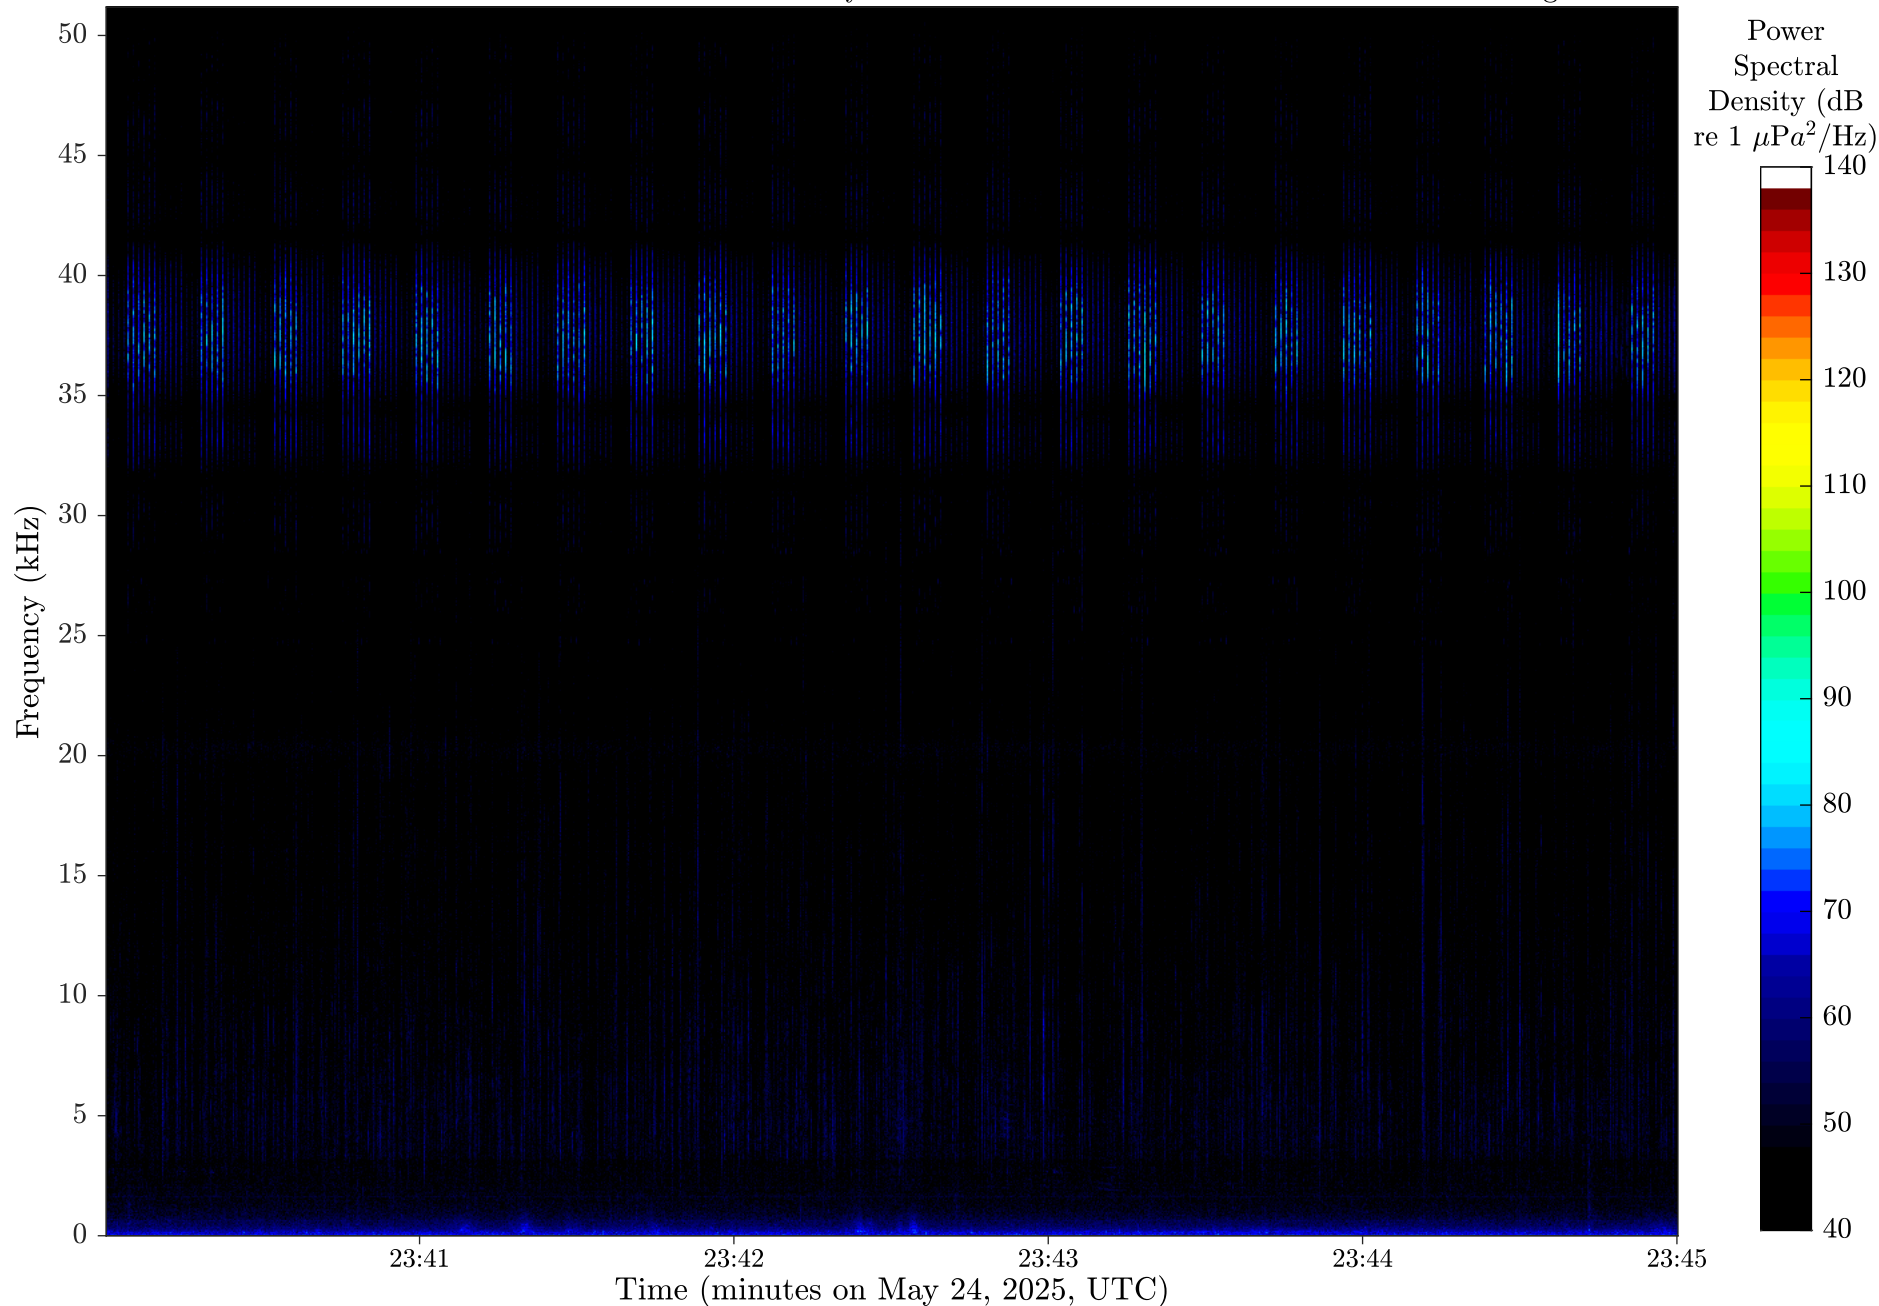


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:40 UTC

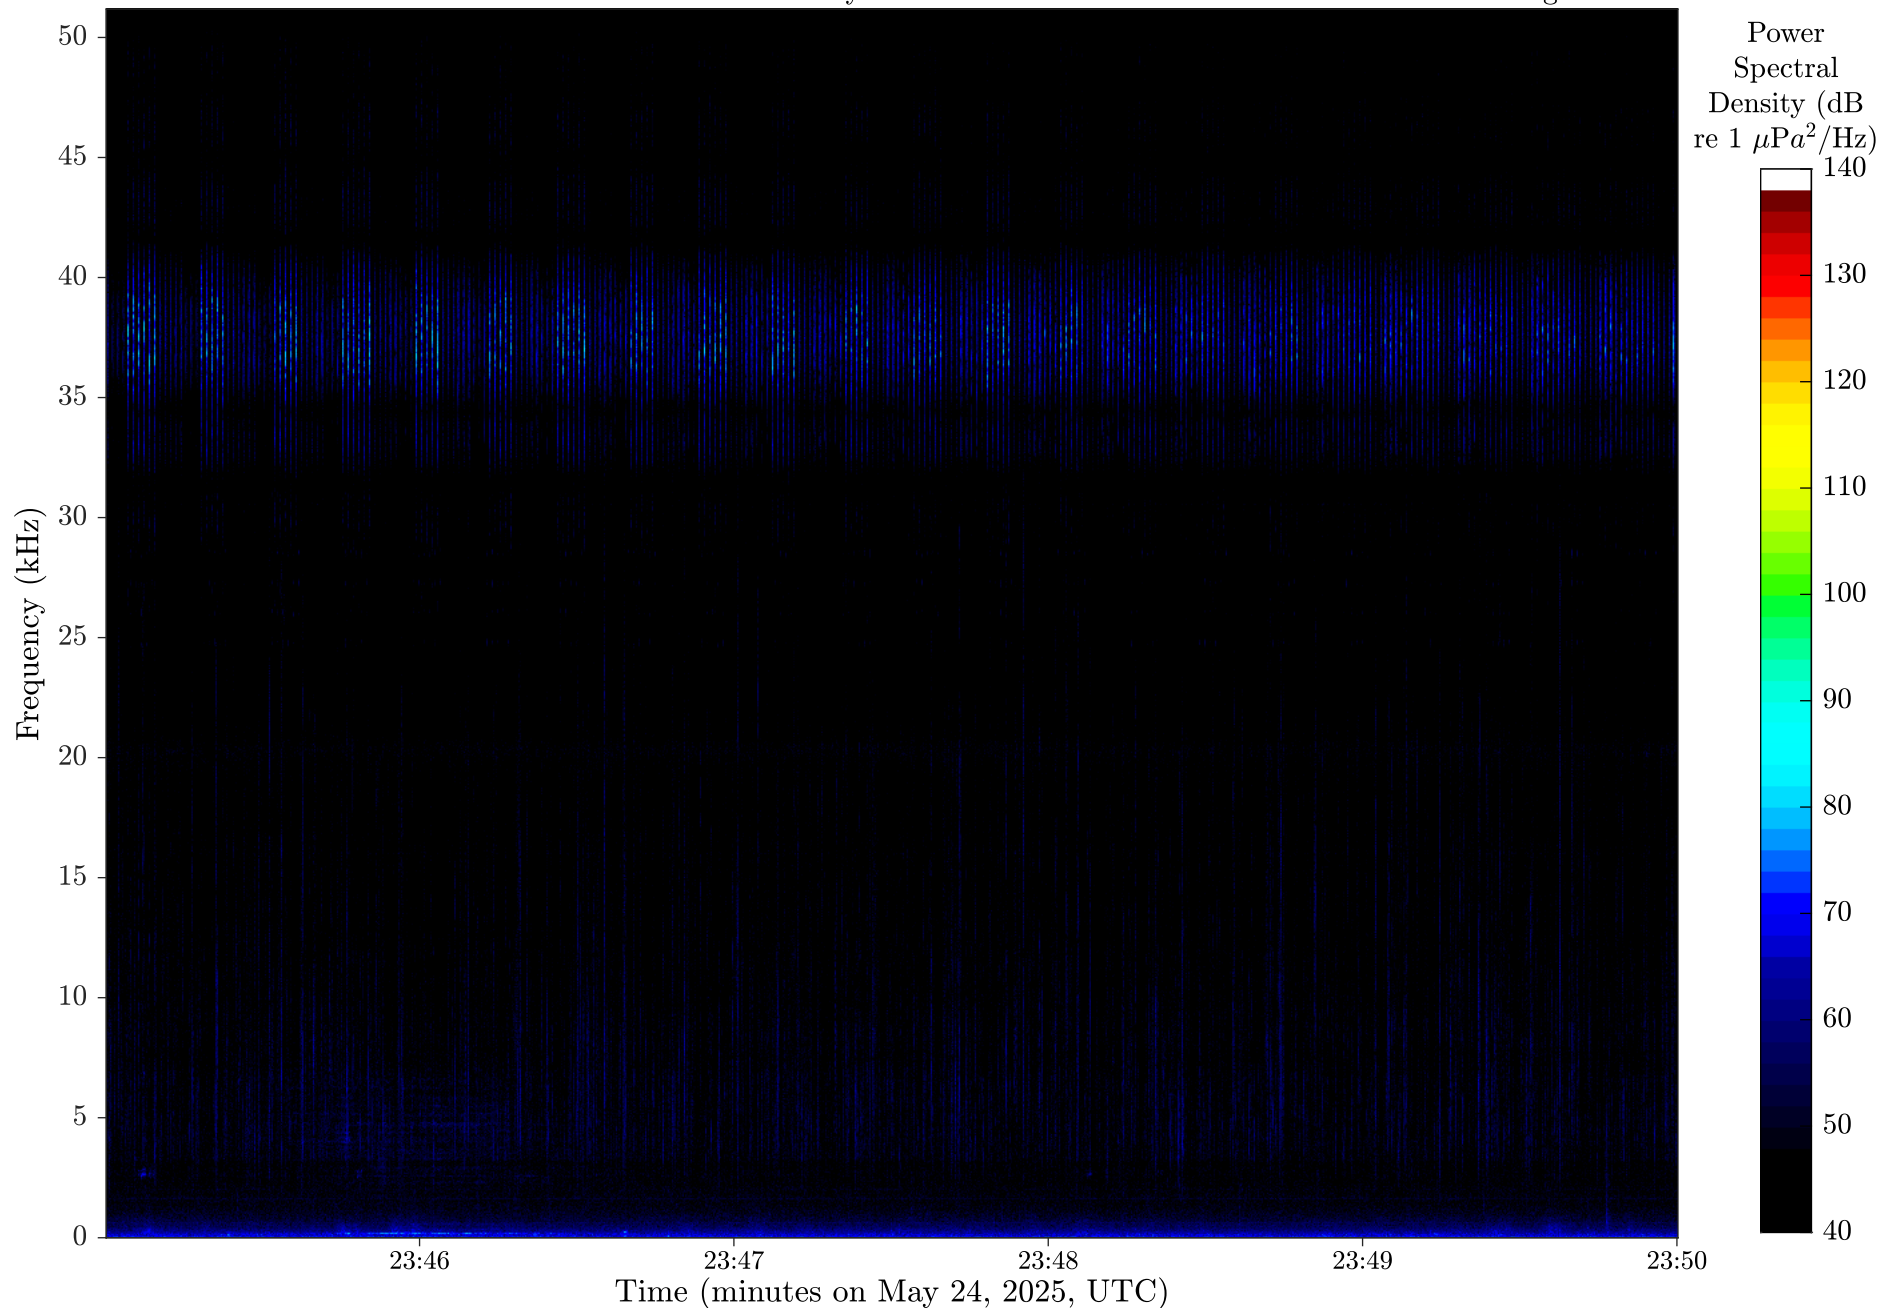

Comments: 34.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:47 UTC

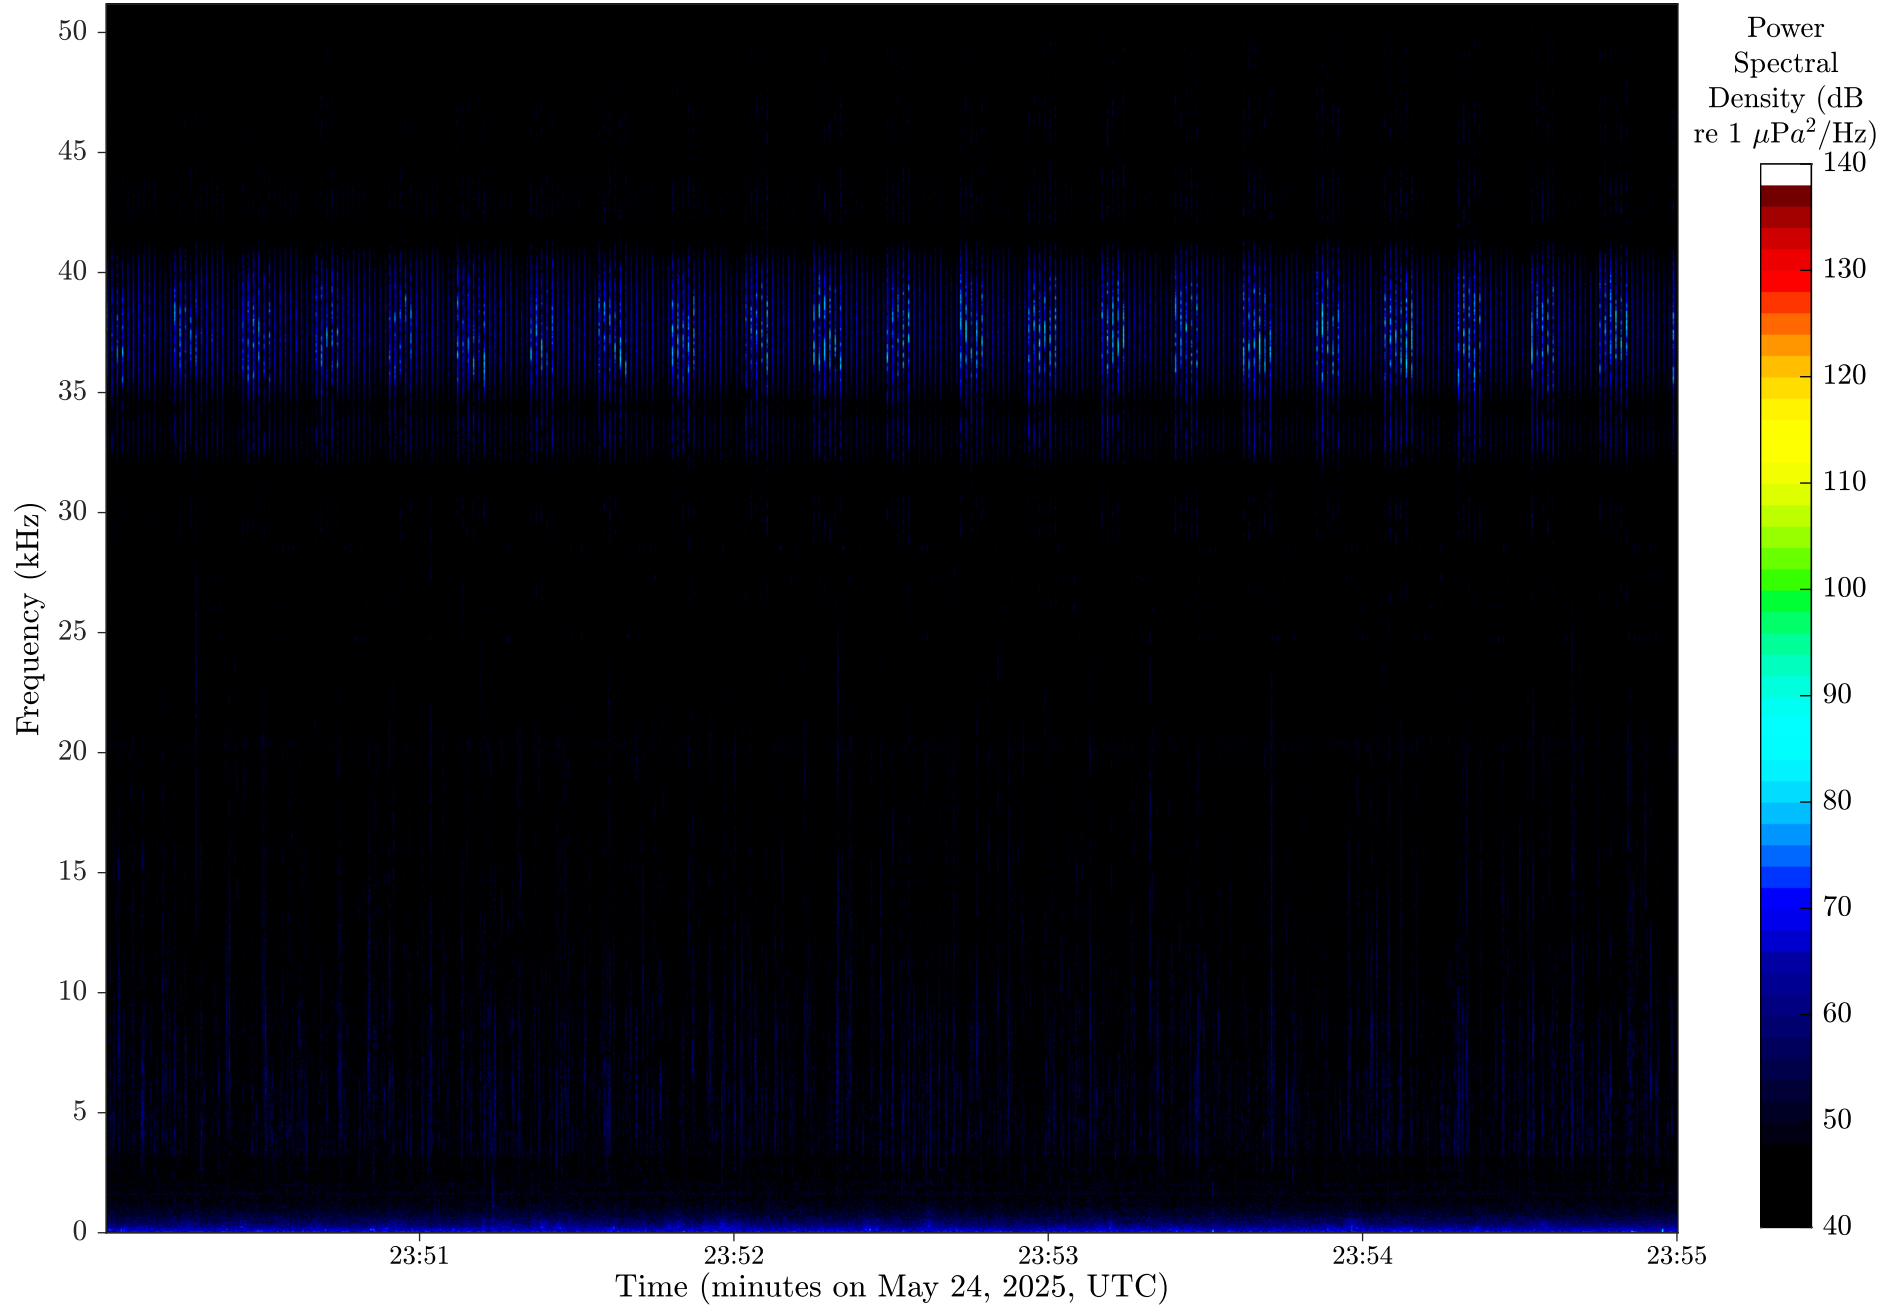

Comments: 34.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:54 UTC

