



Comments: 31.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:14:54 UTC

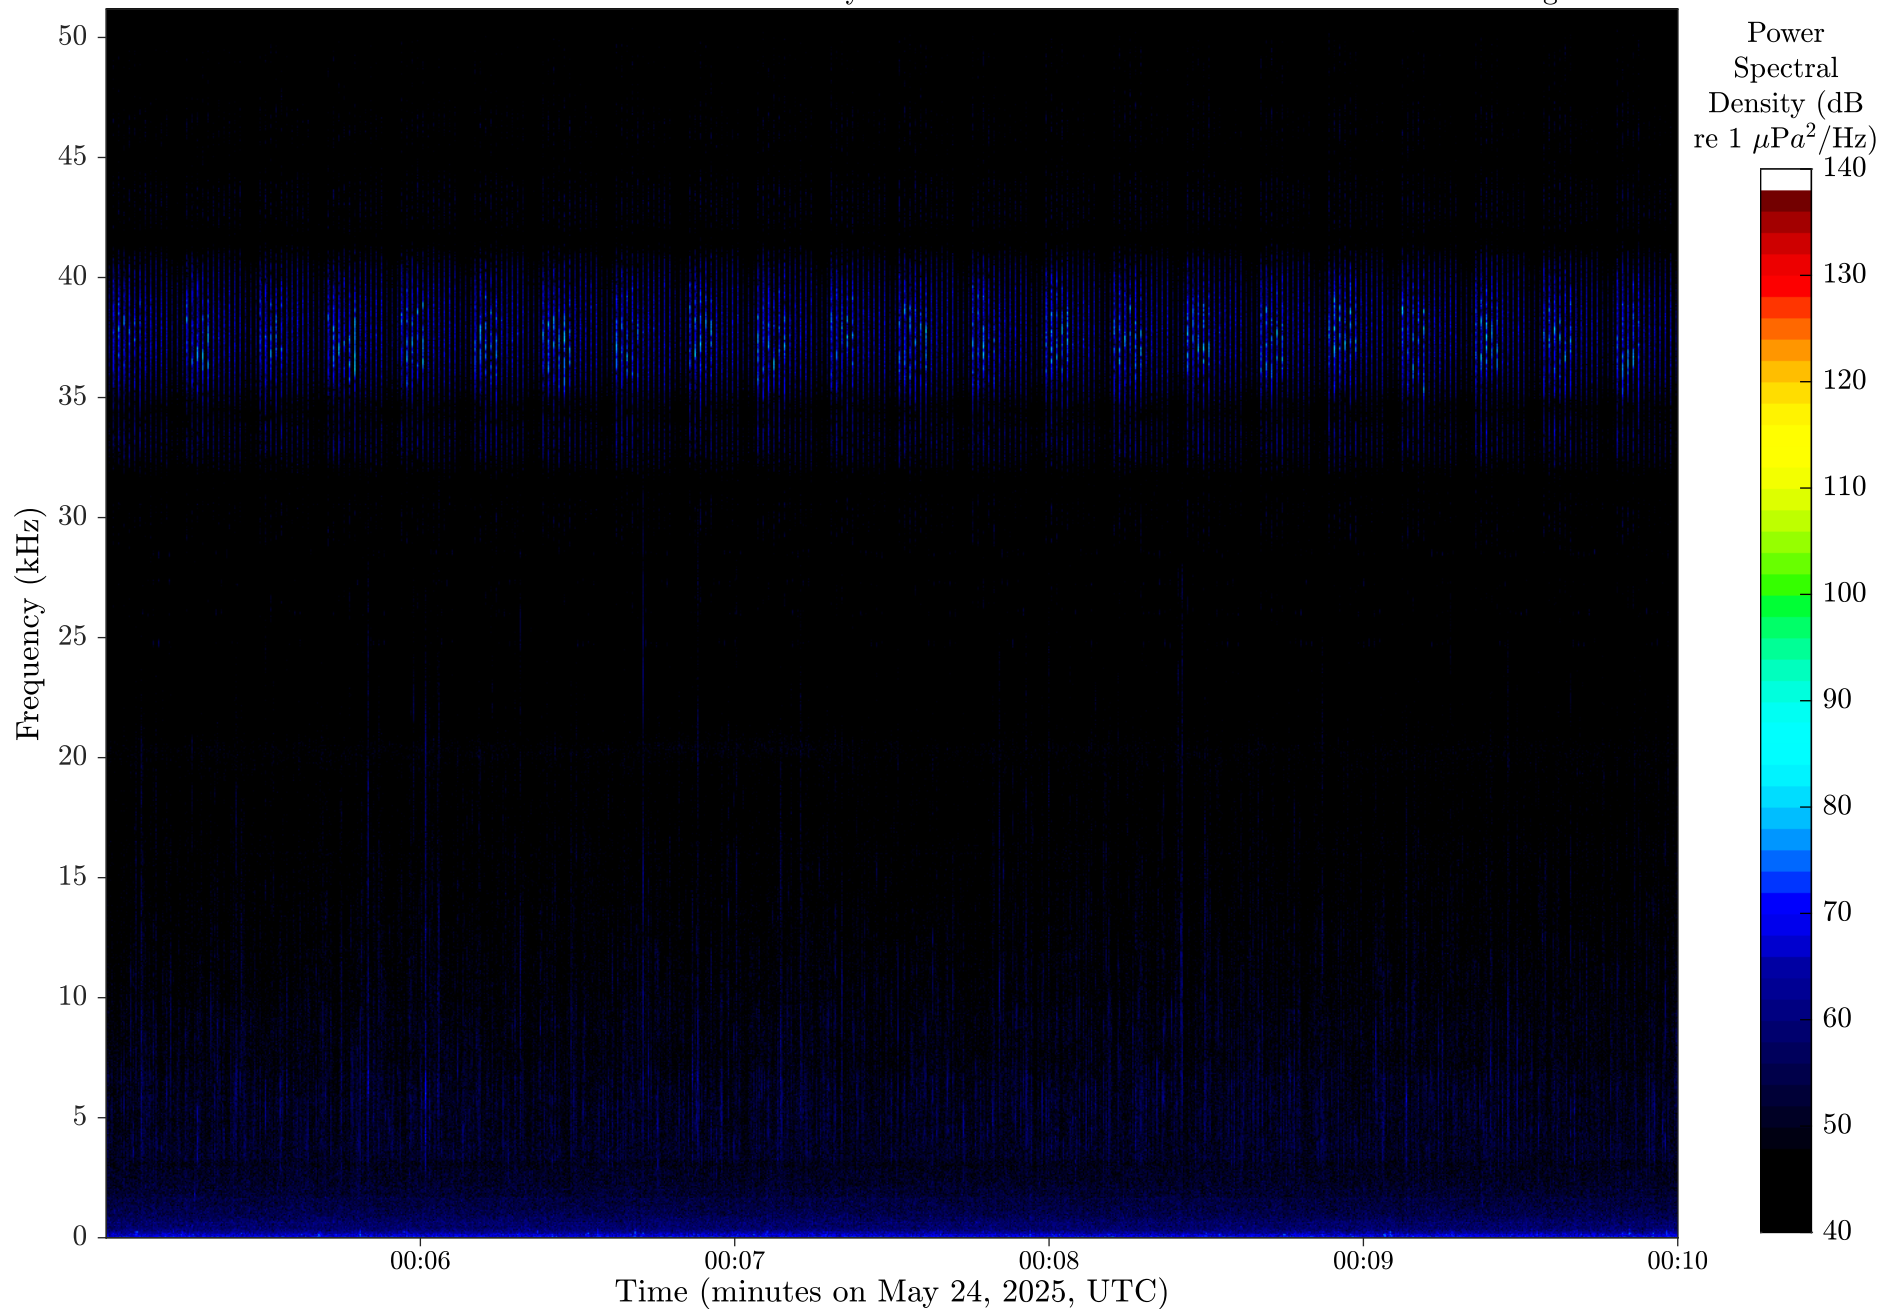


Comments: 32.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:15:04 UTC

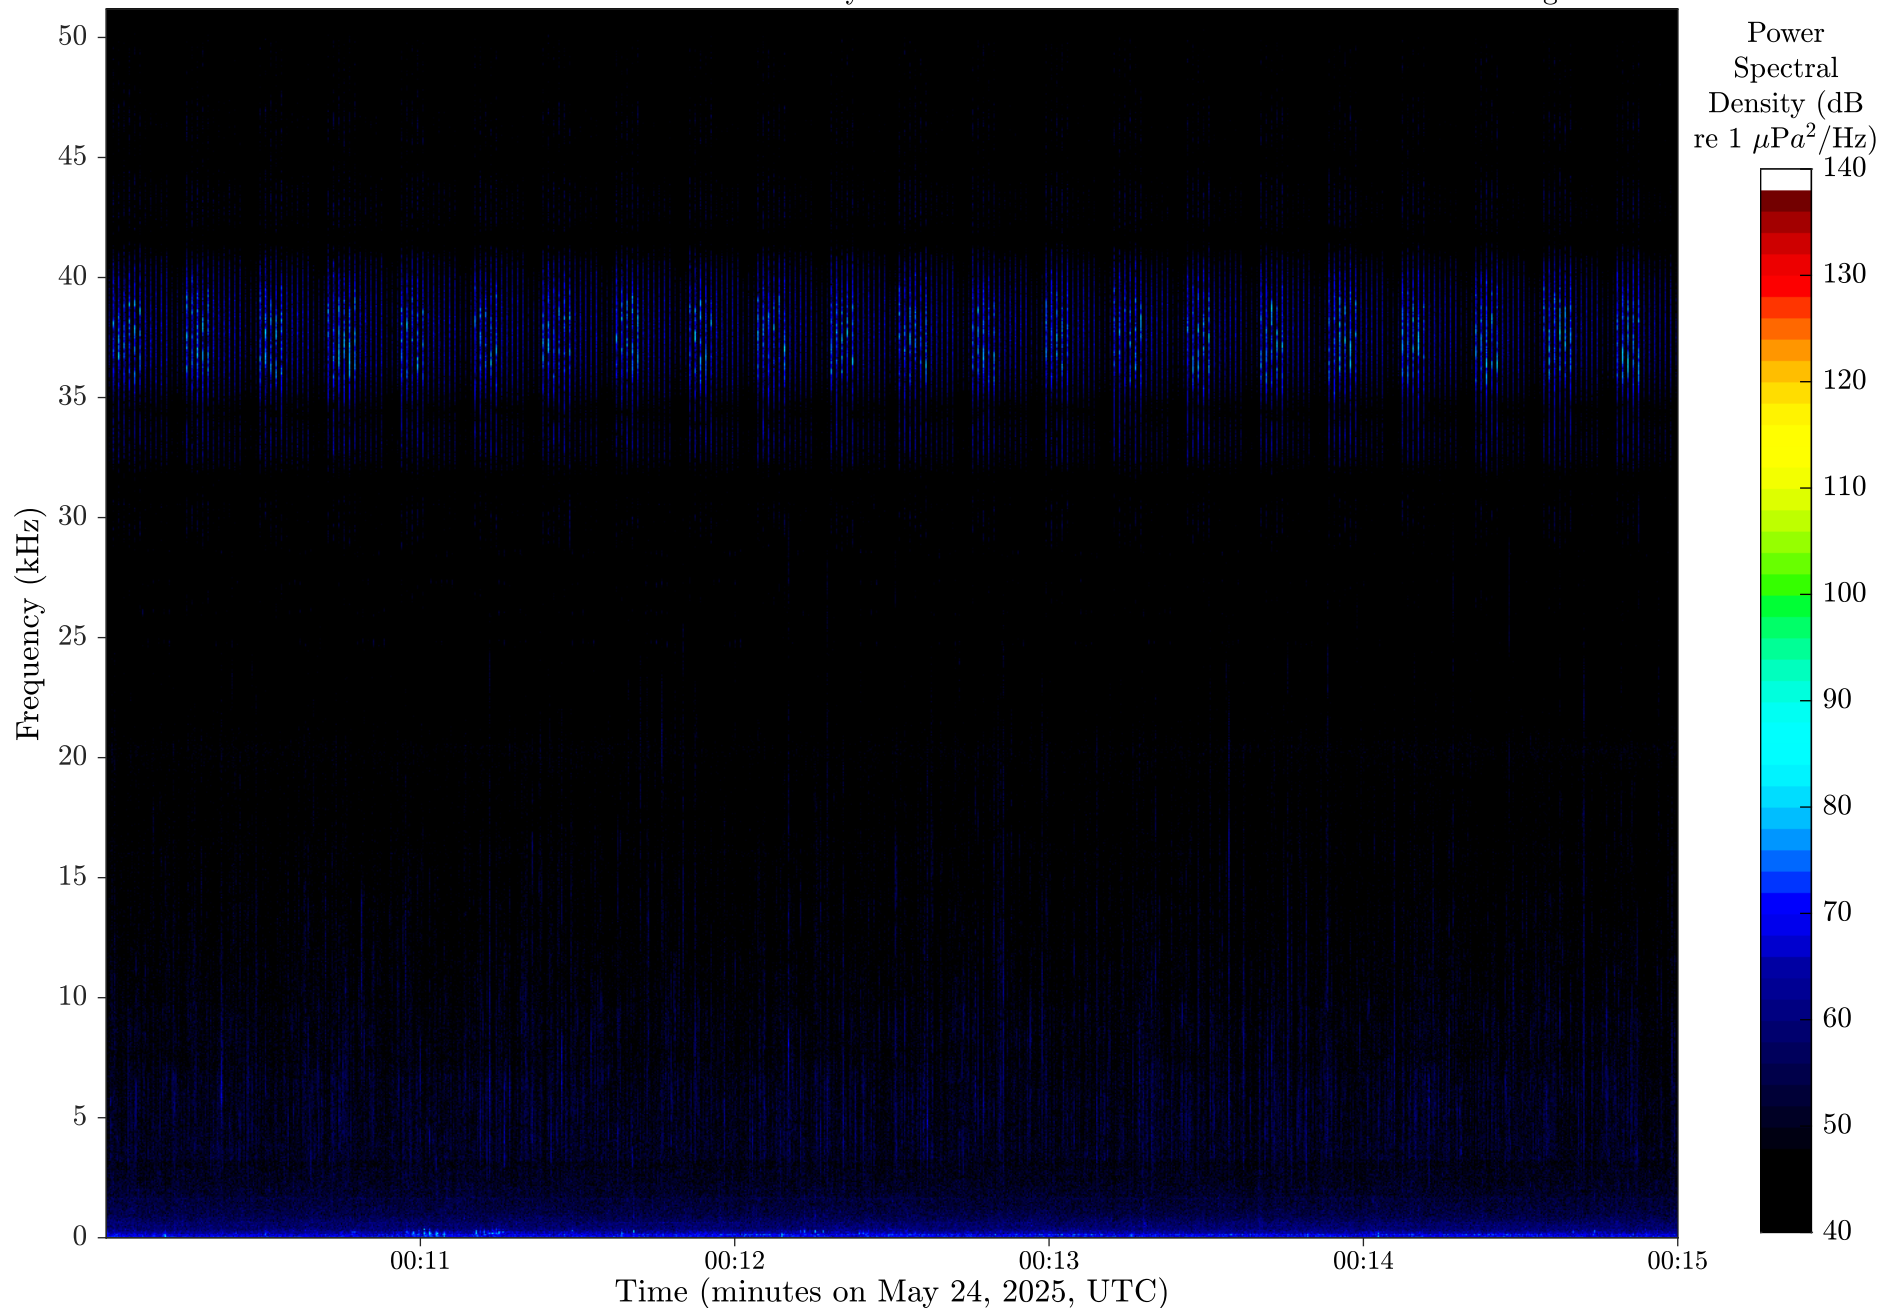


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:15:13 UTC

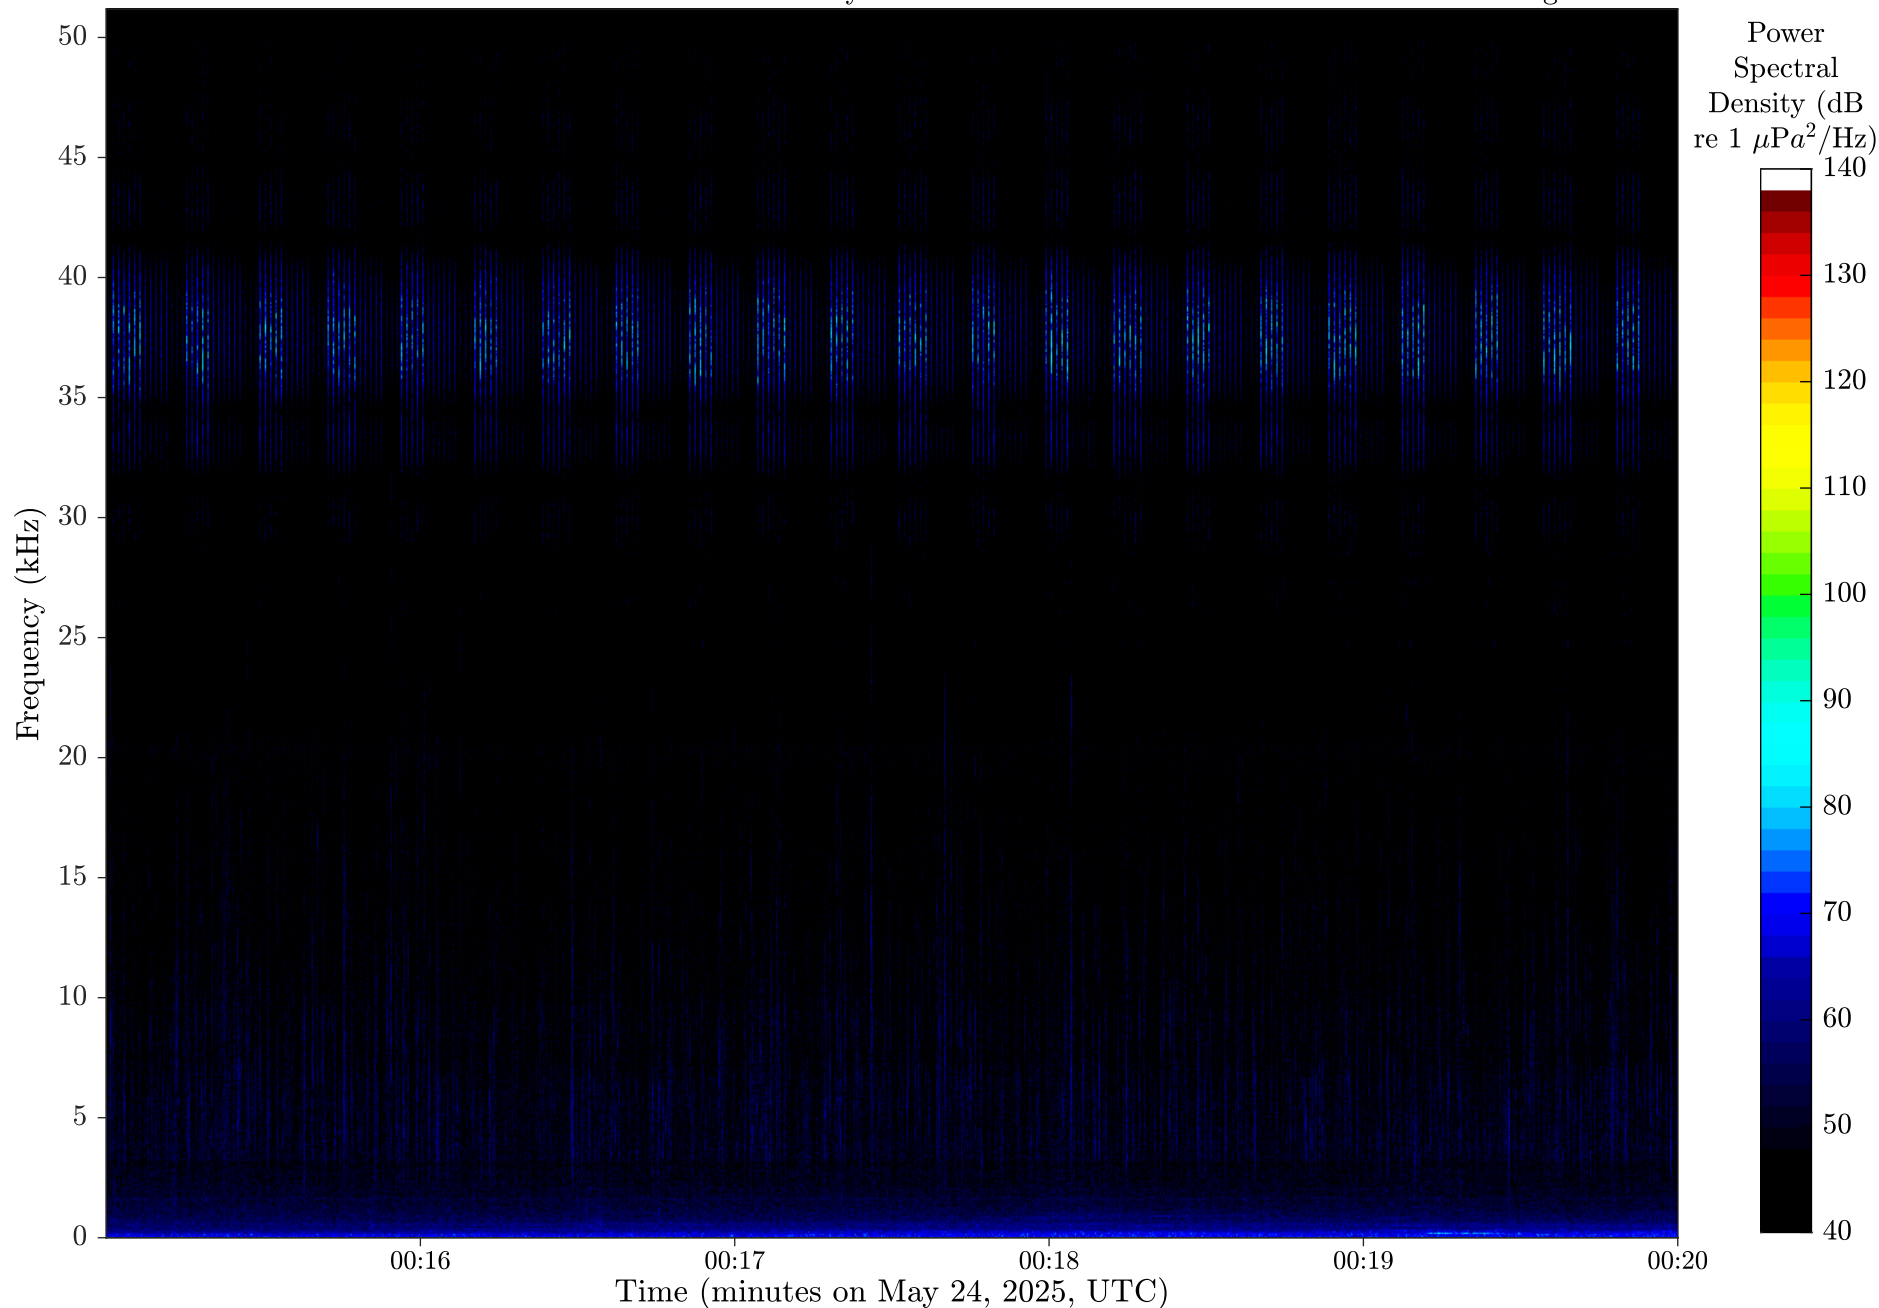


Comments: 35.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:15:22 UTC

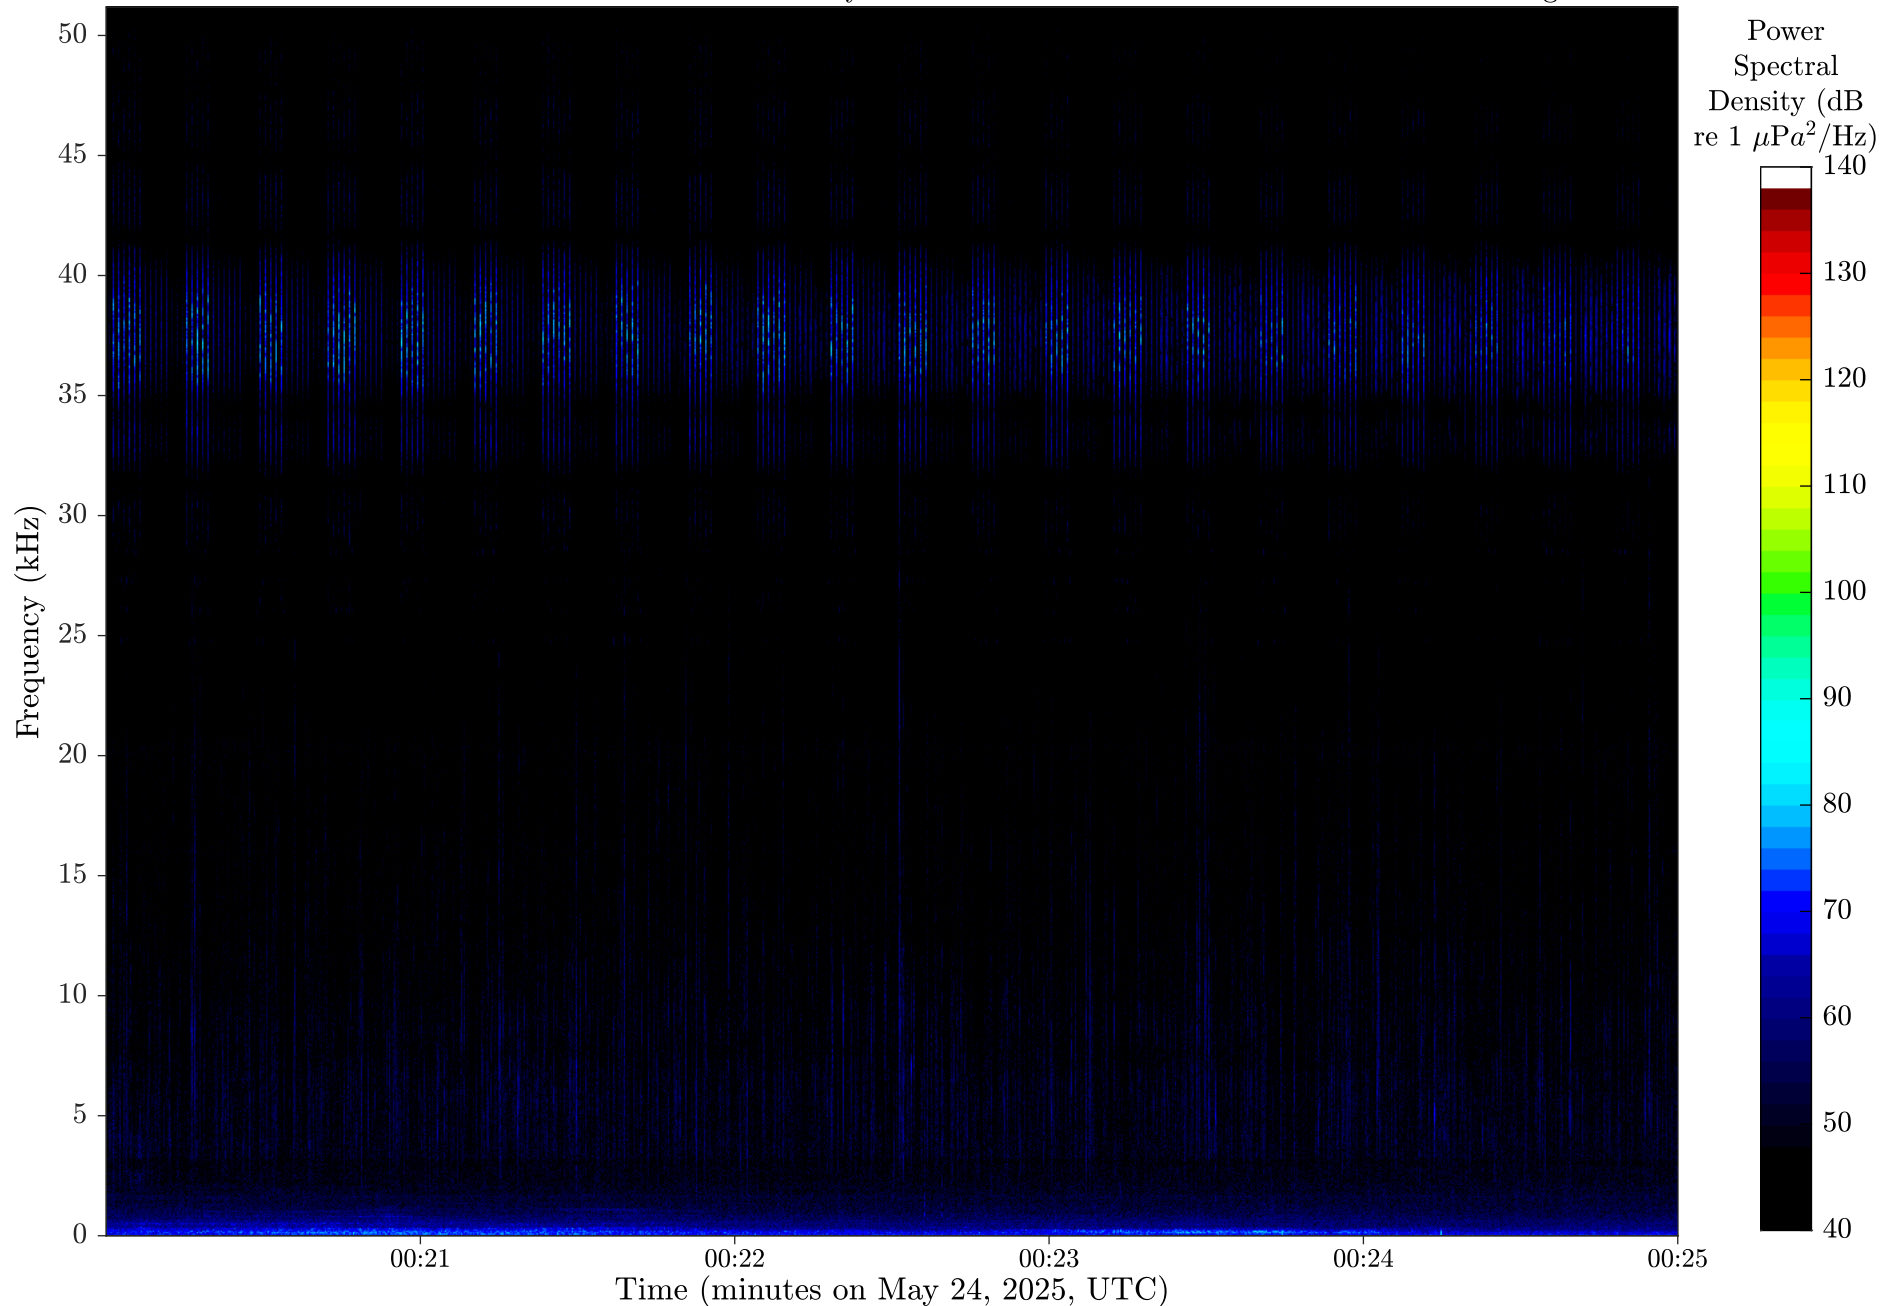

Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:15:30 UTC

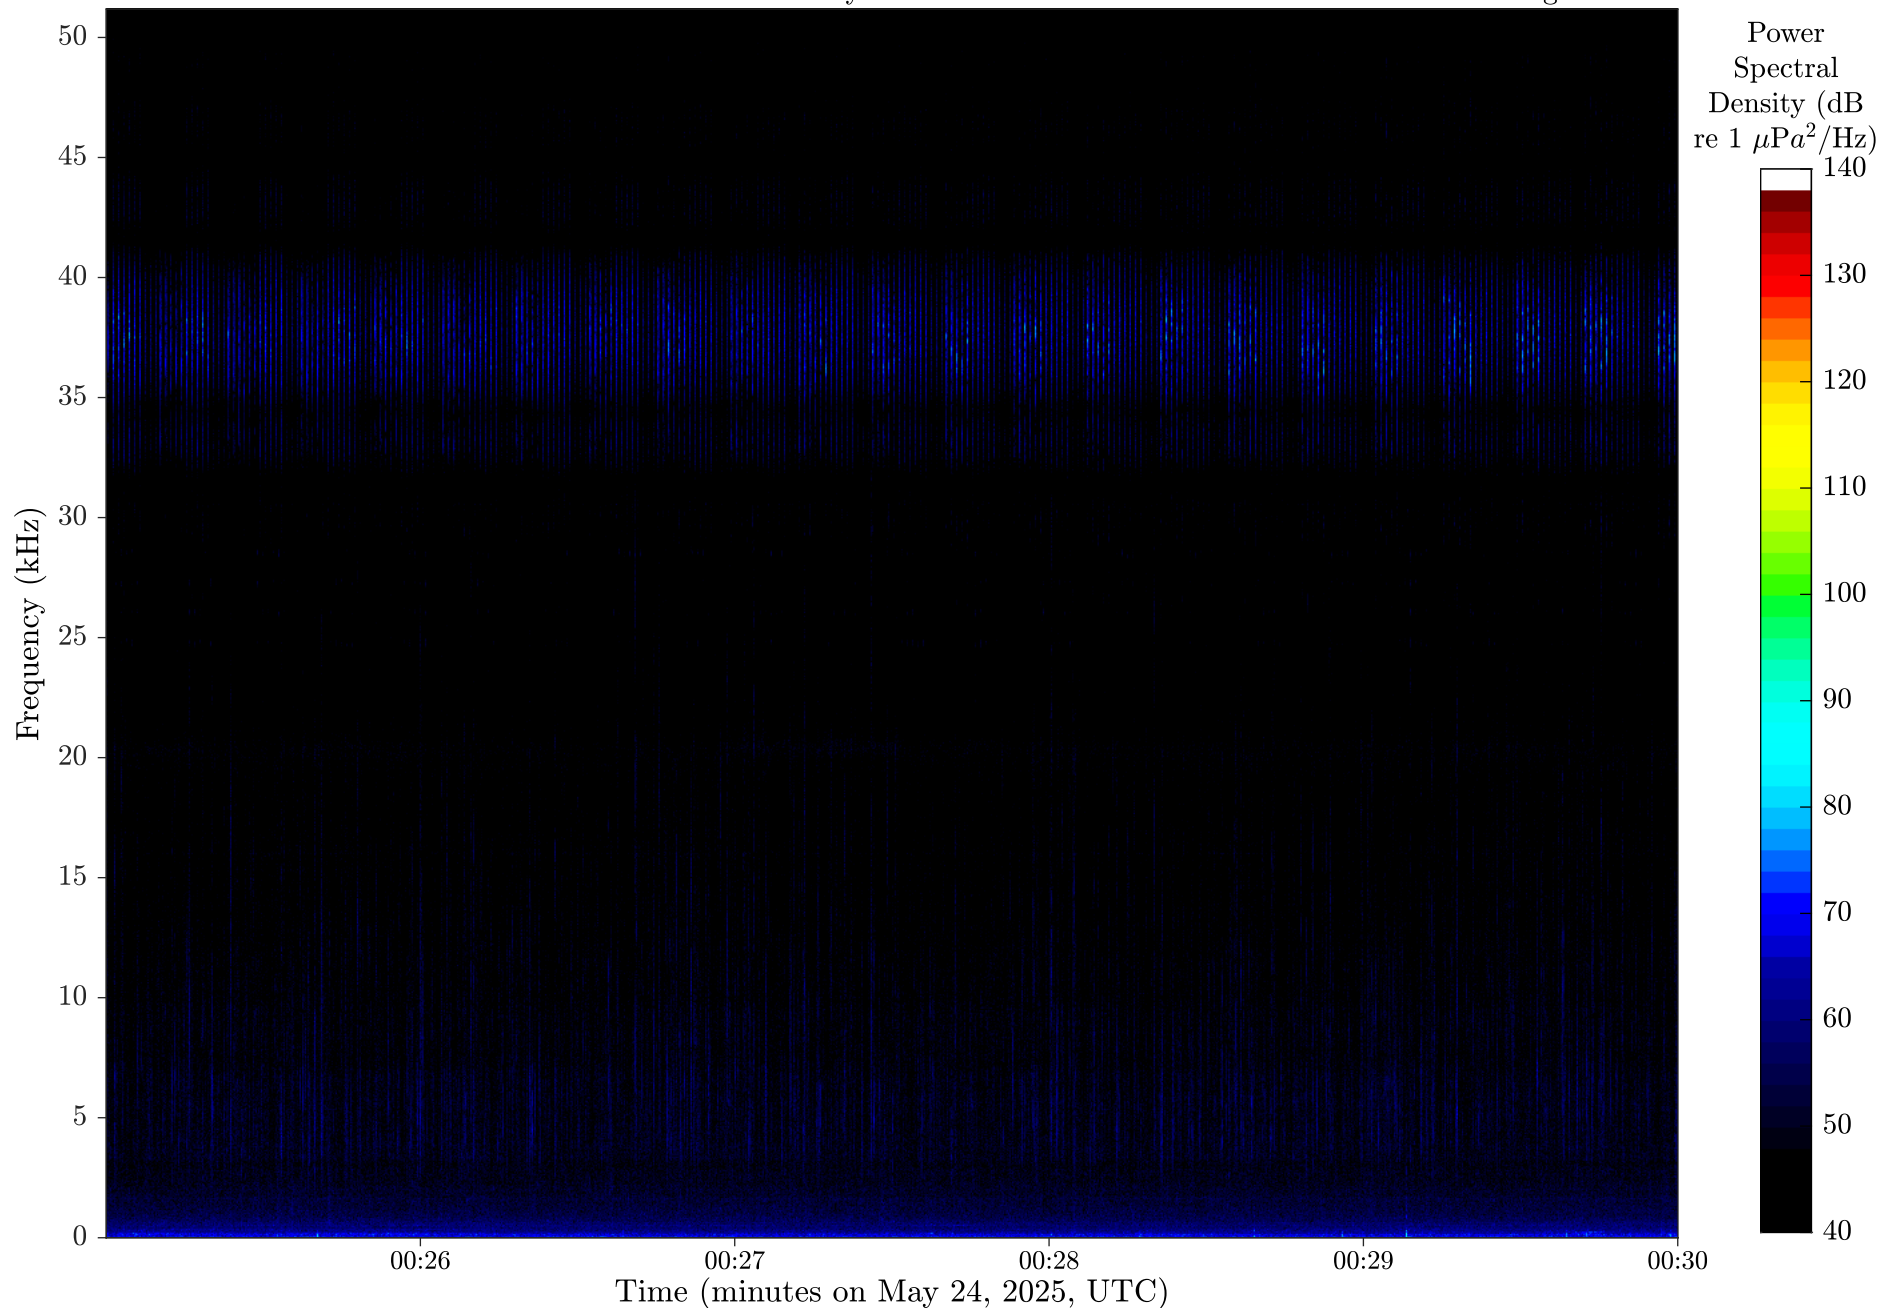


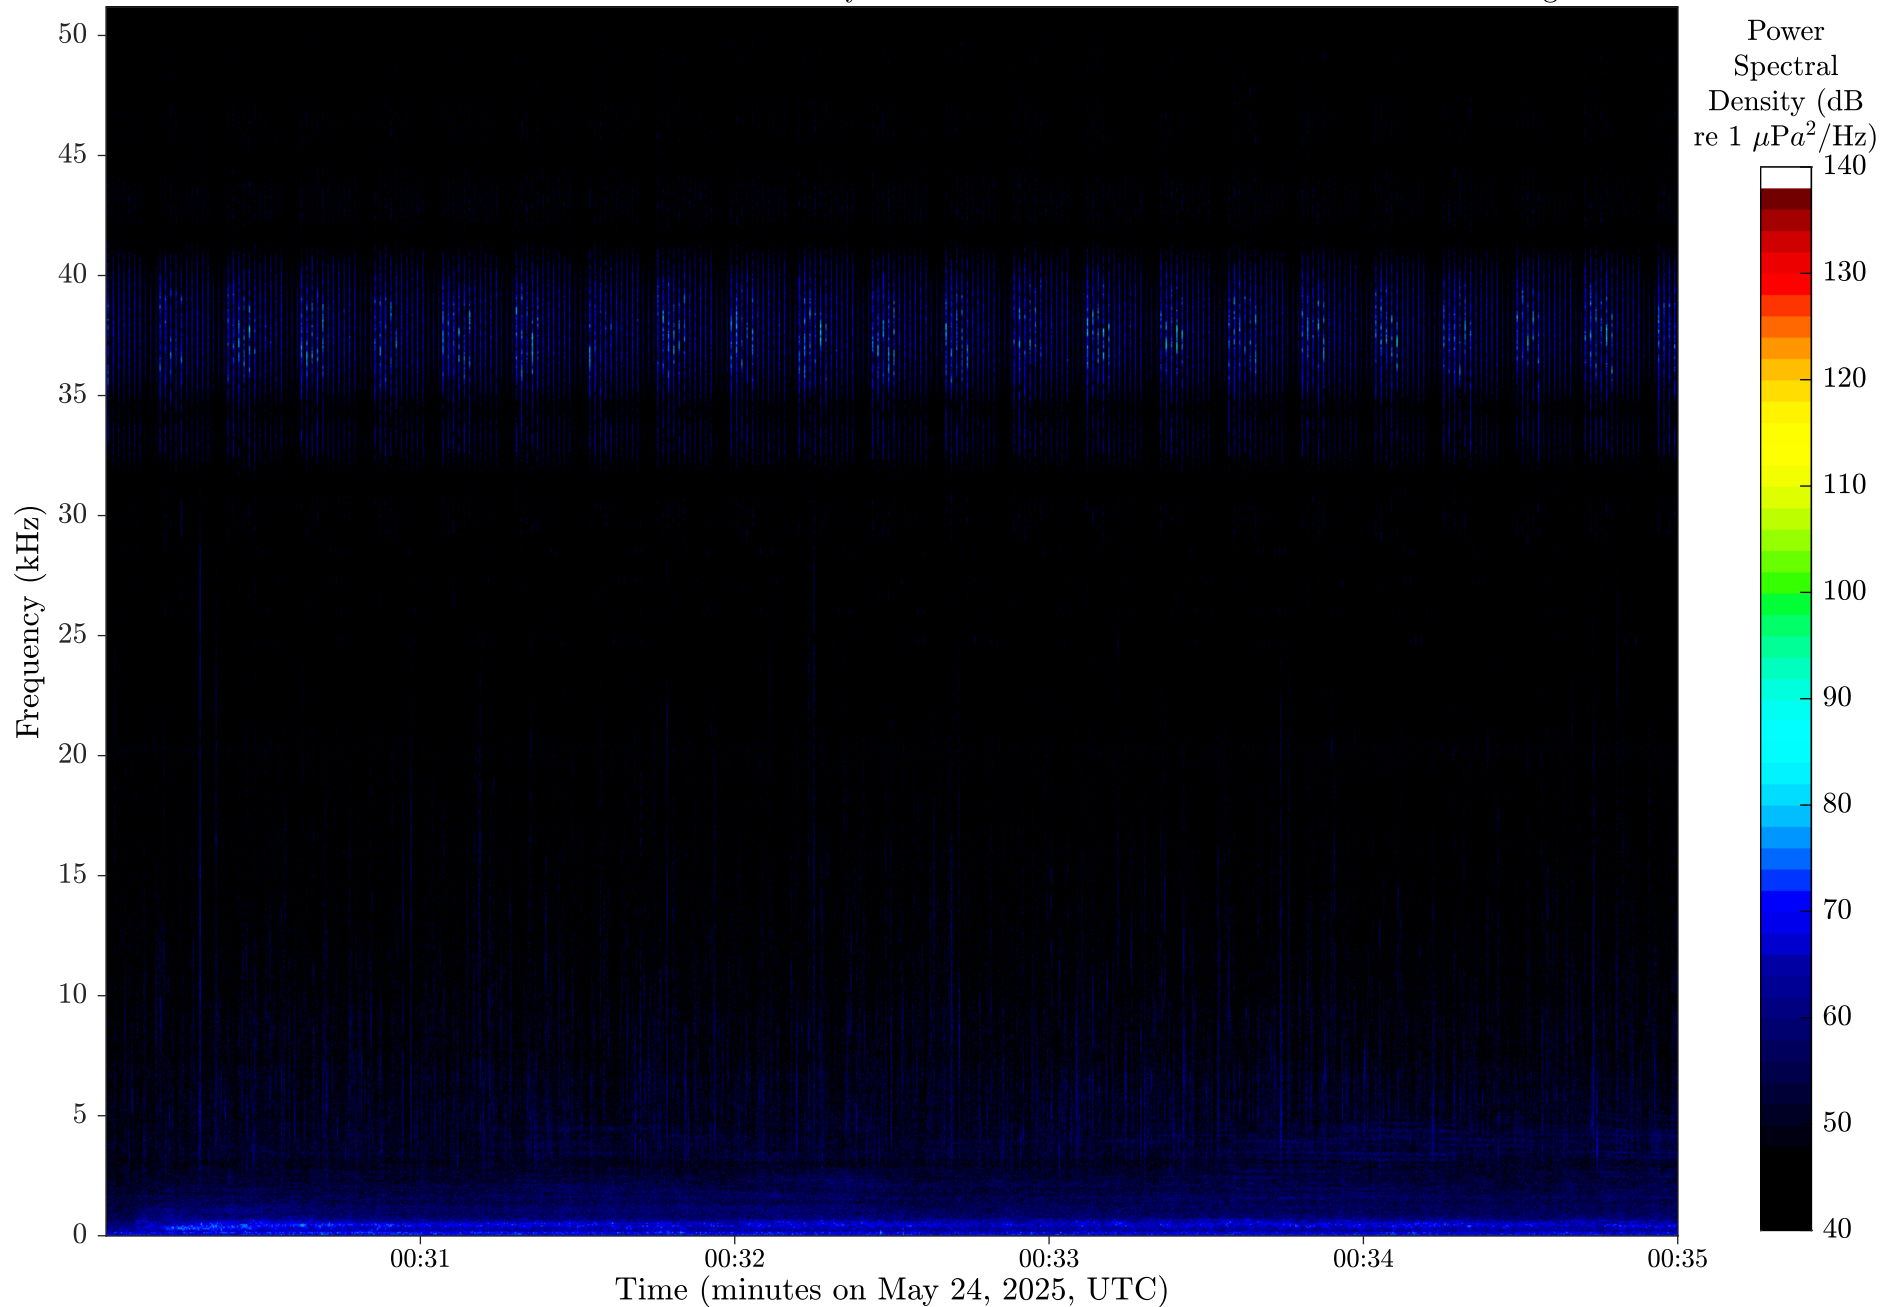

Comments: 33.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:15:47 UTC

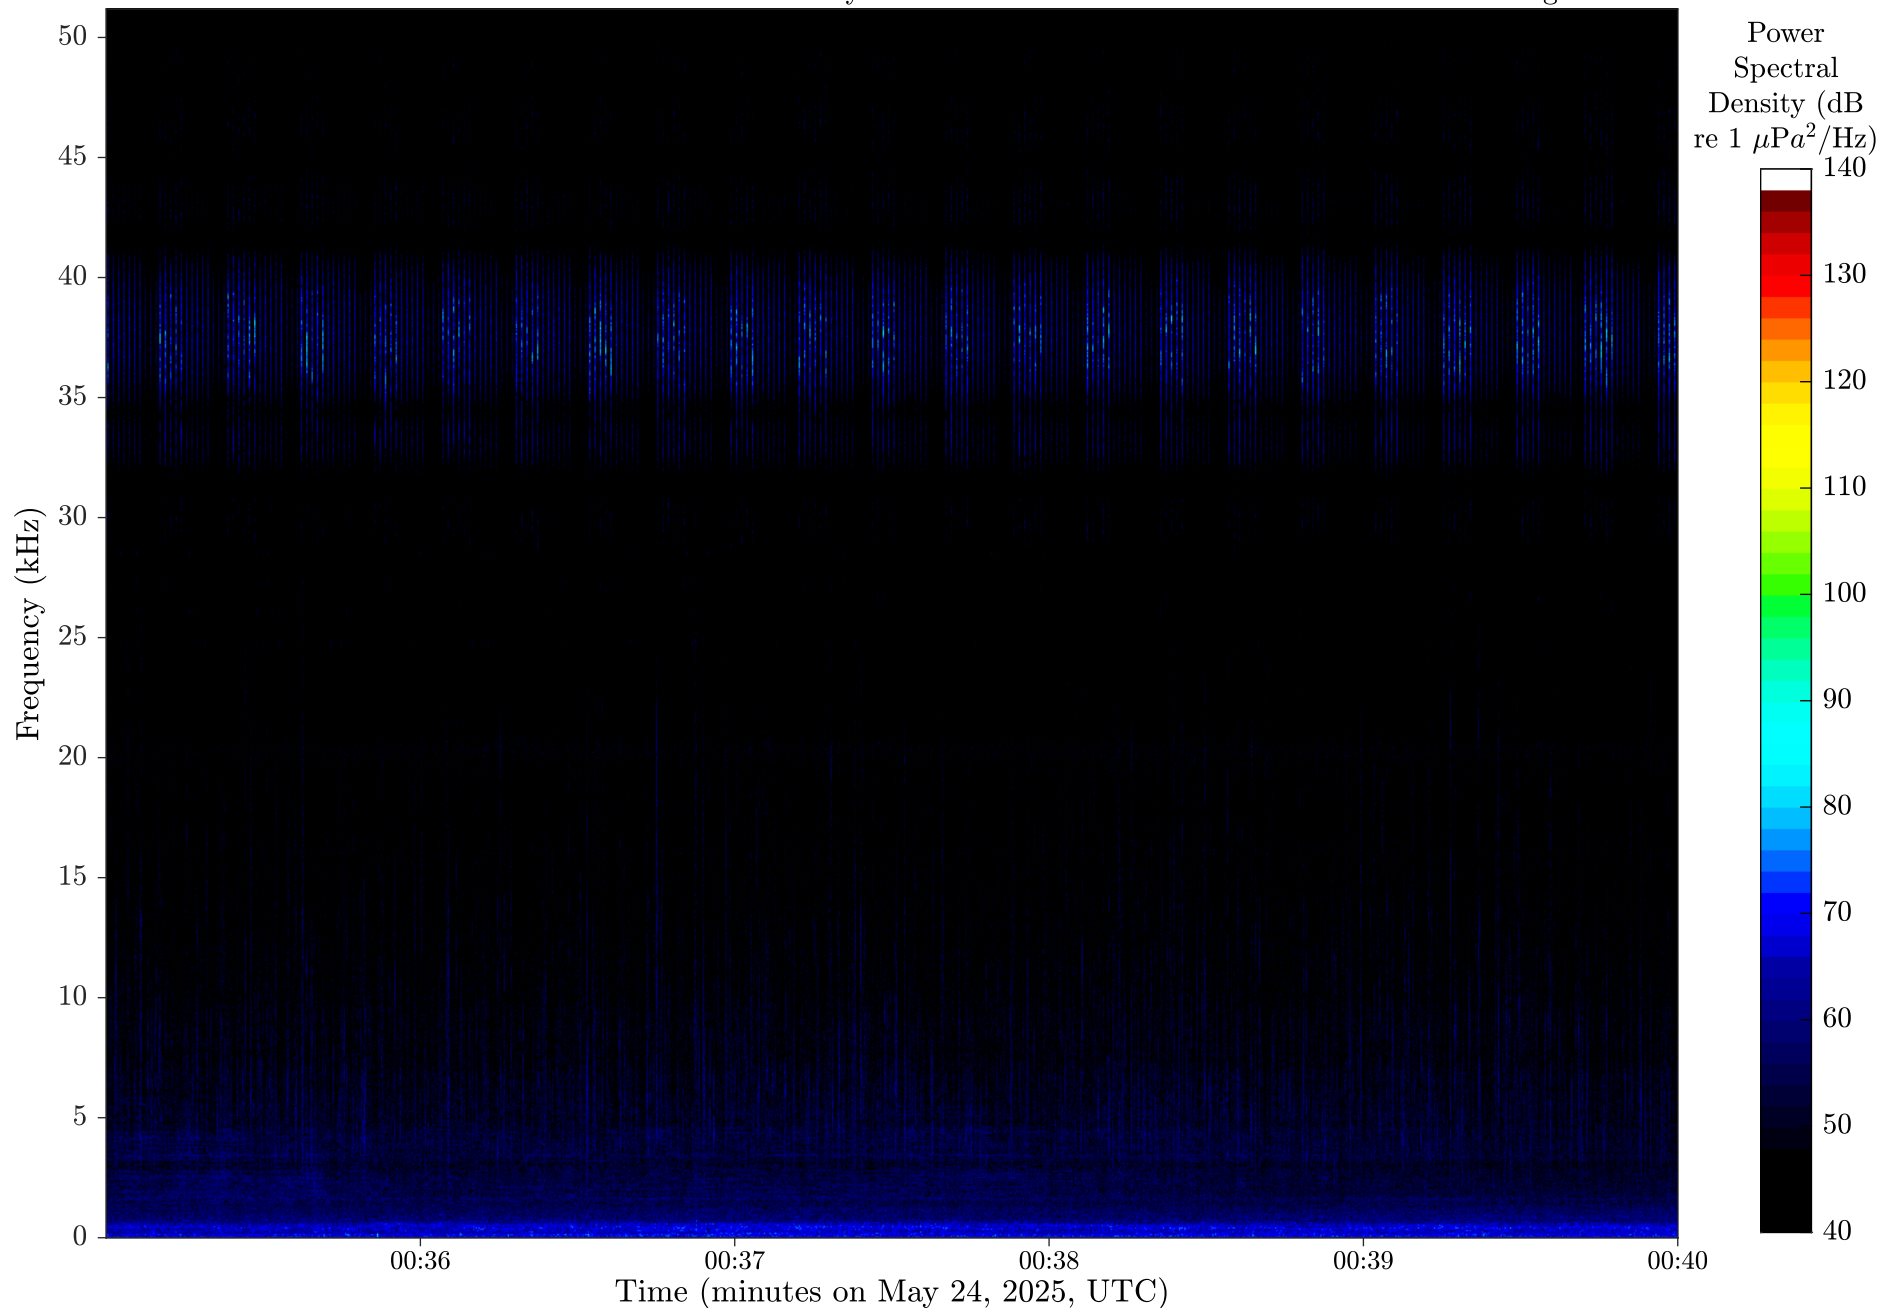

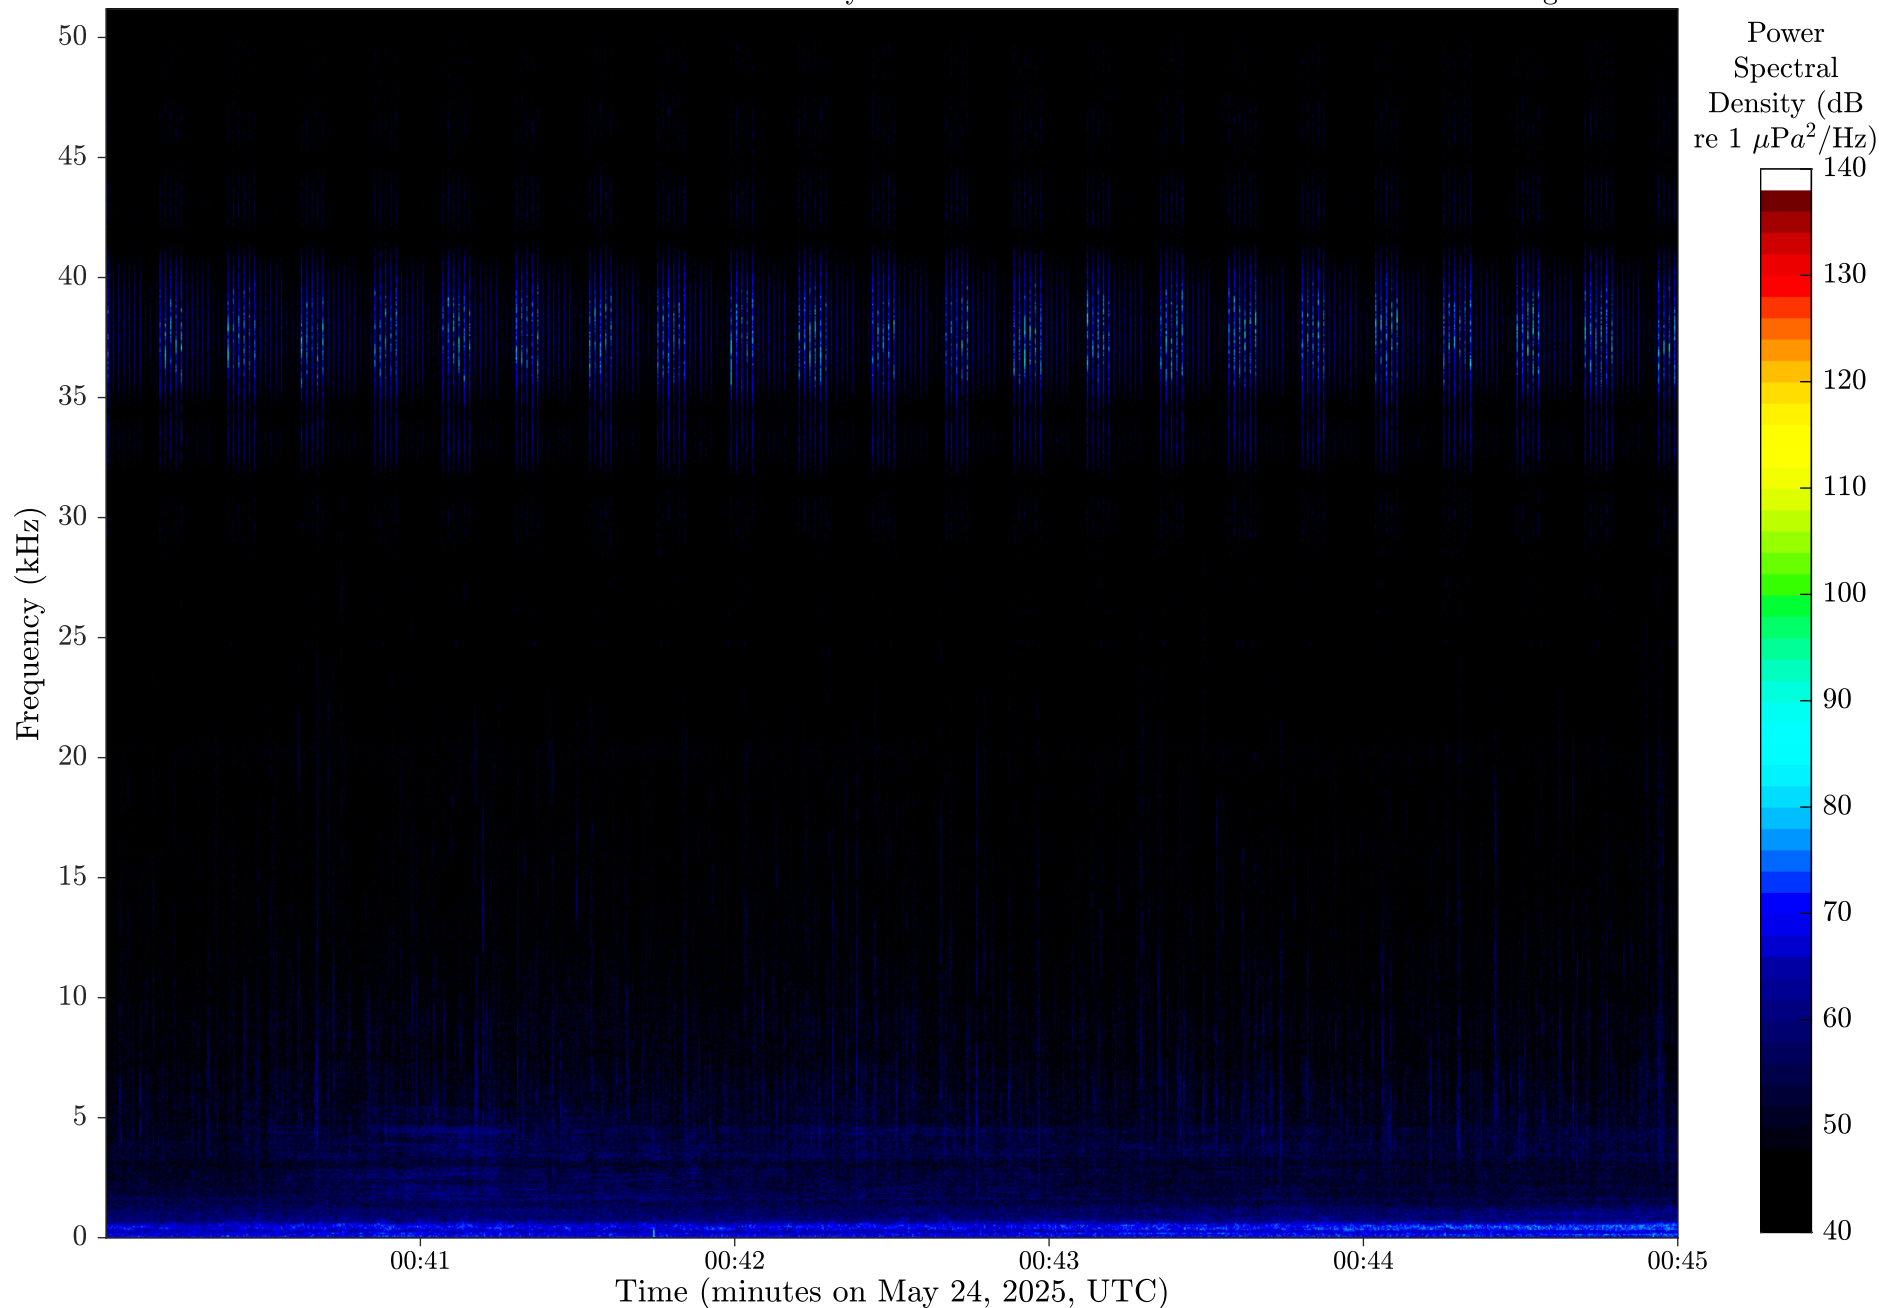


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:16:04 UTC

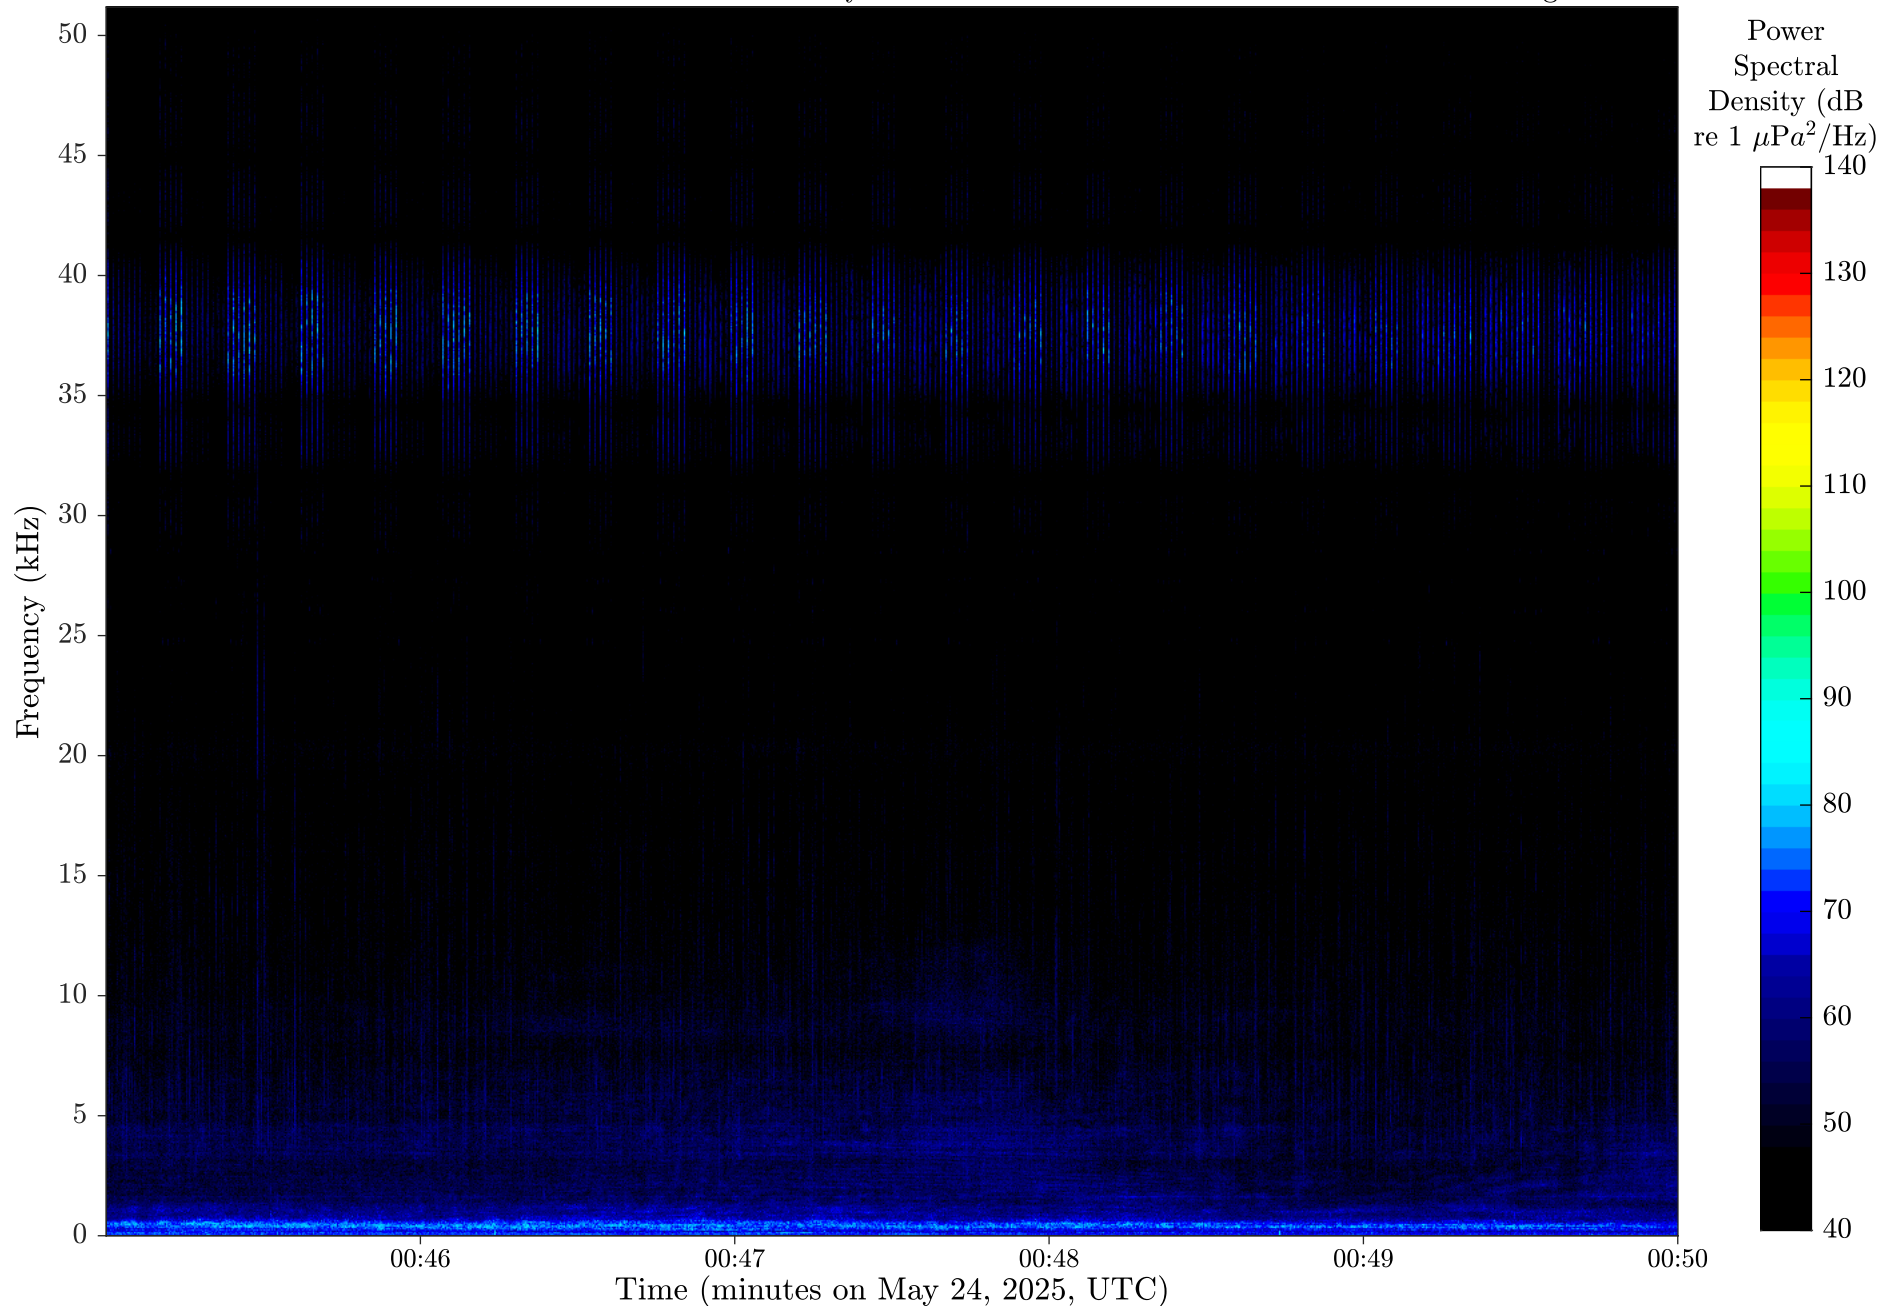

Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:16:12 UTC

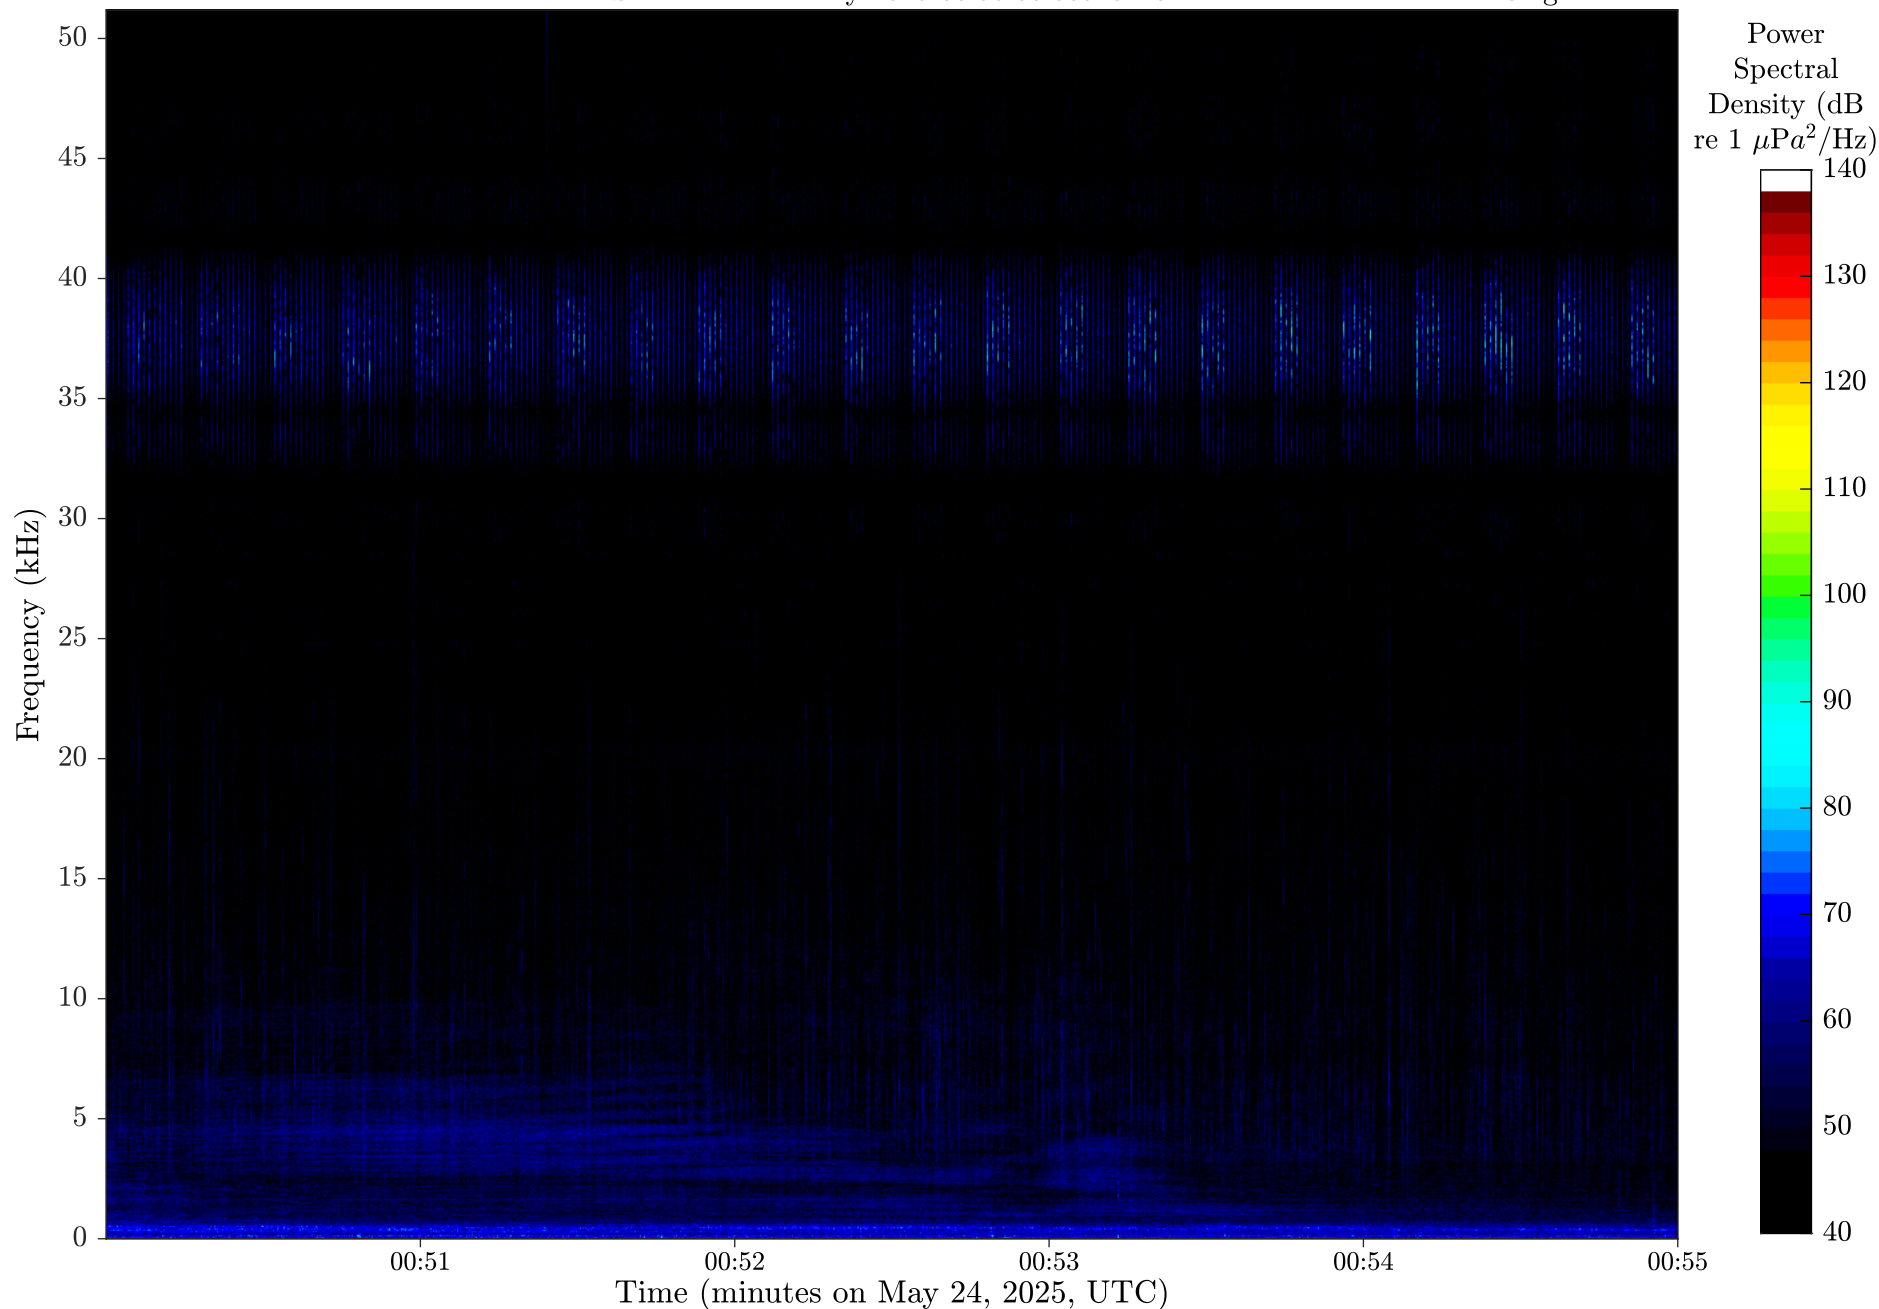

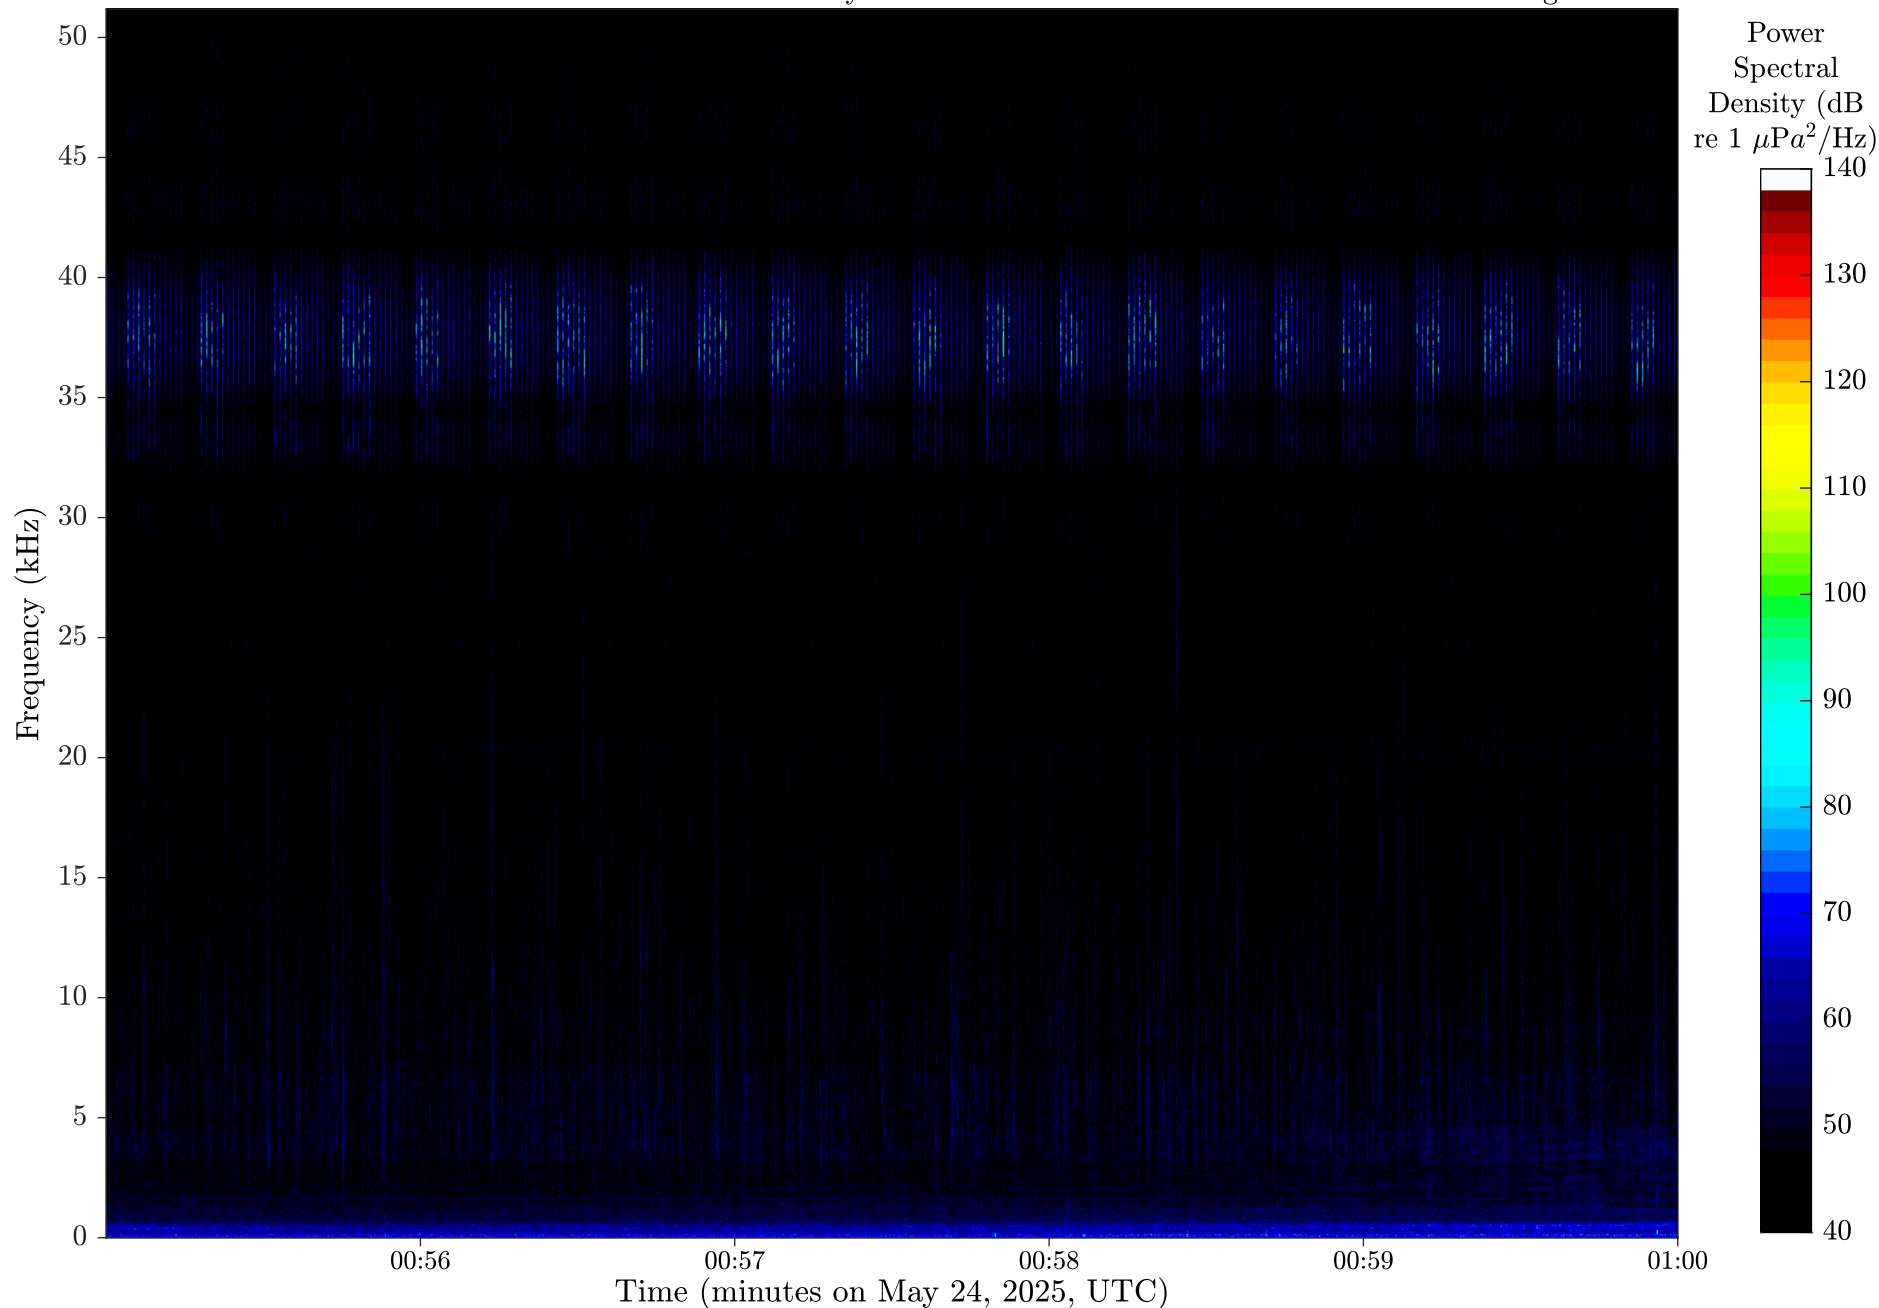


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:16:28 UTC

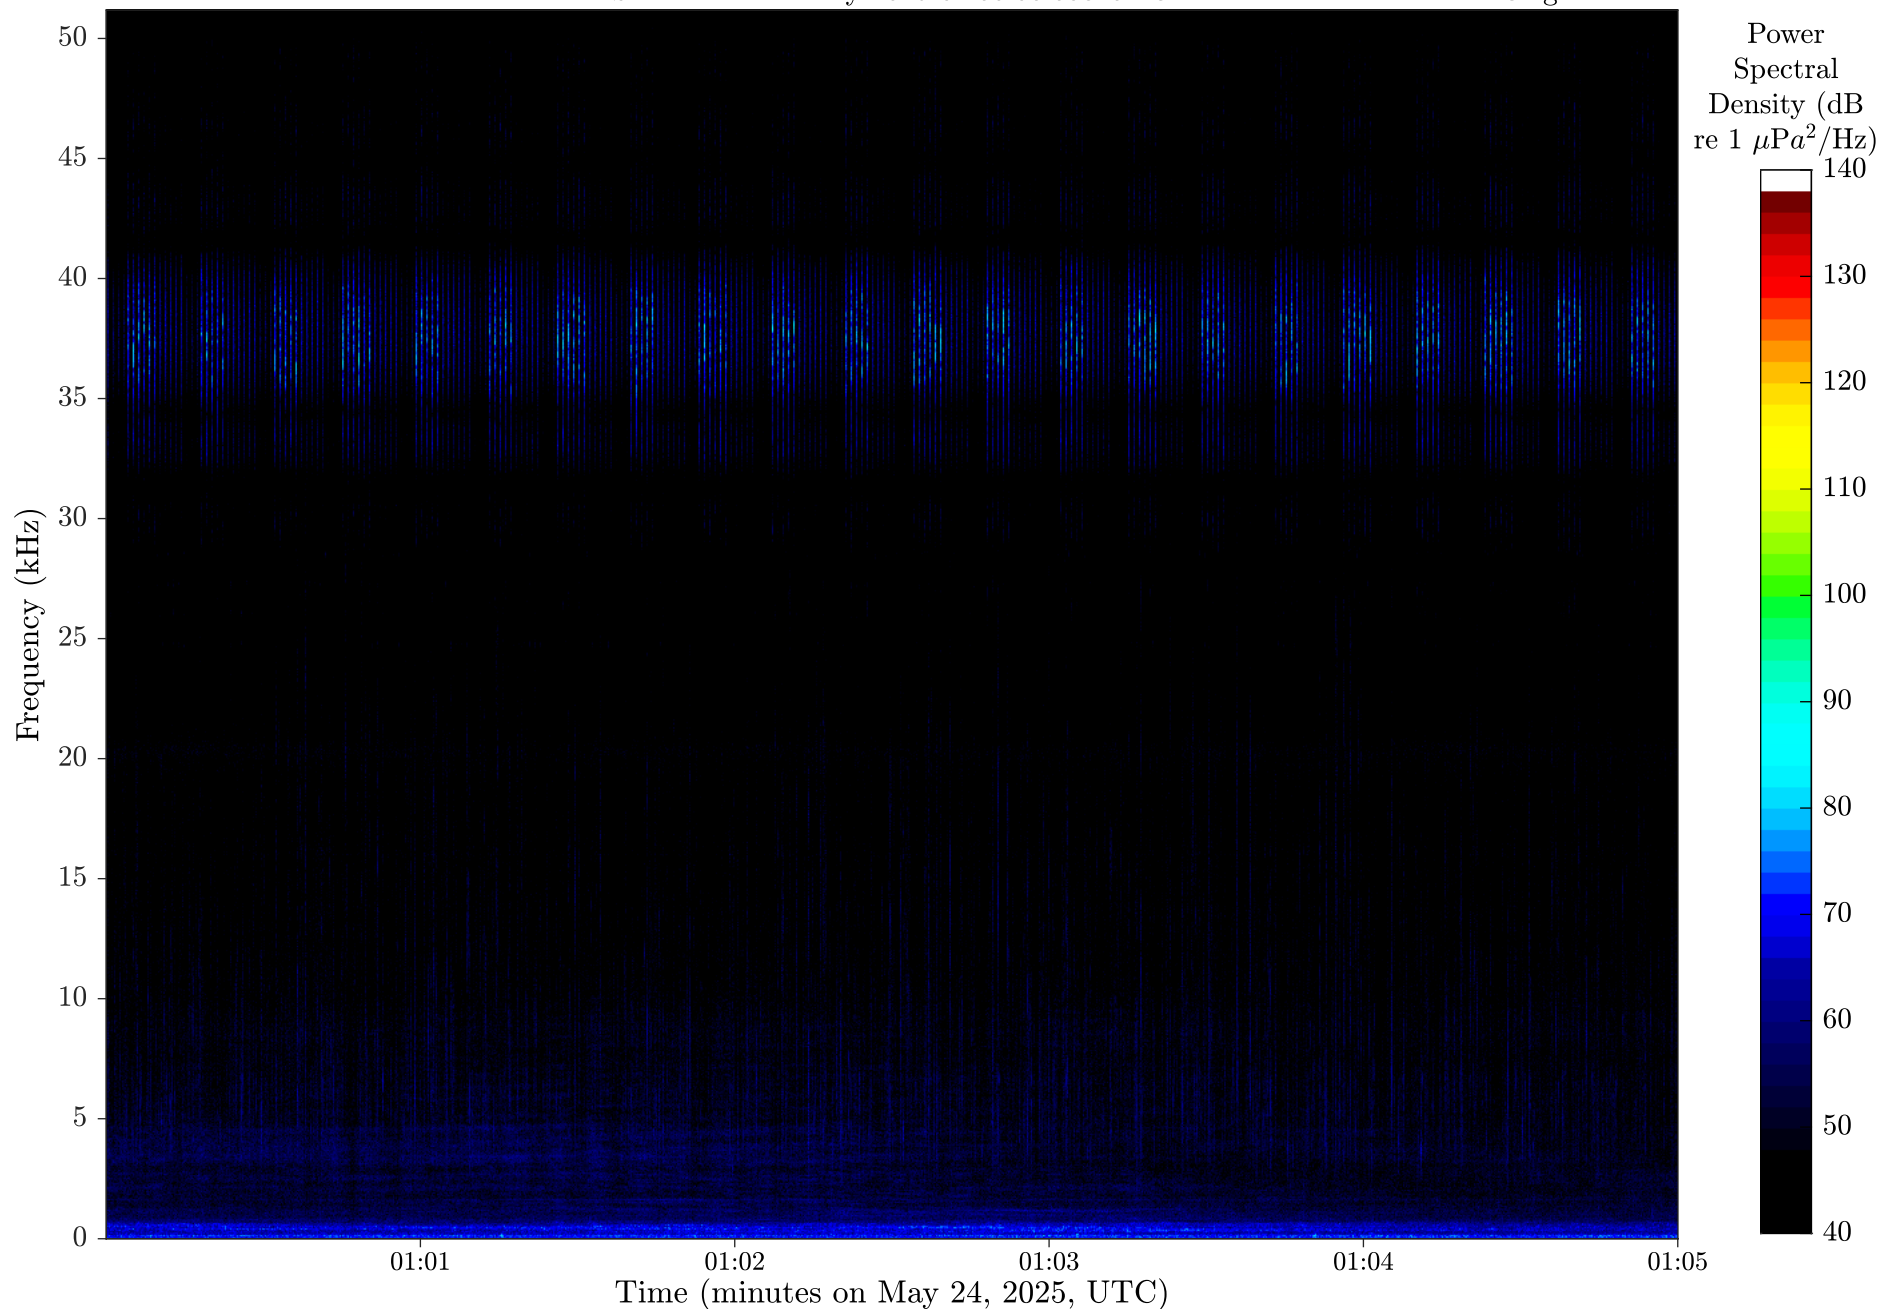

Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:16:36 UTC

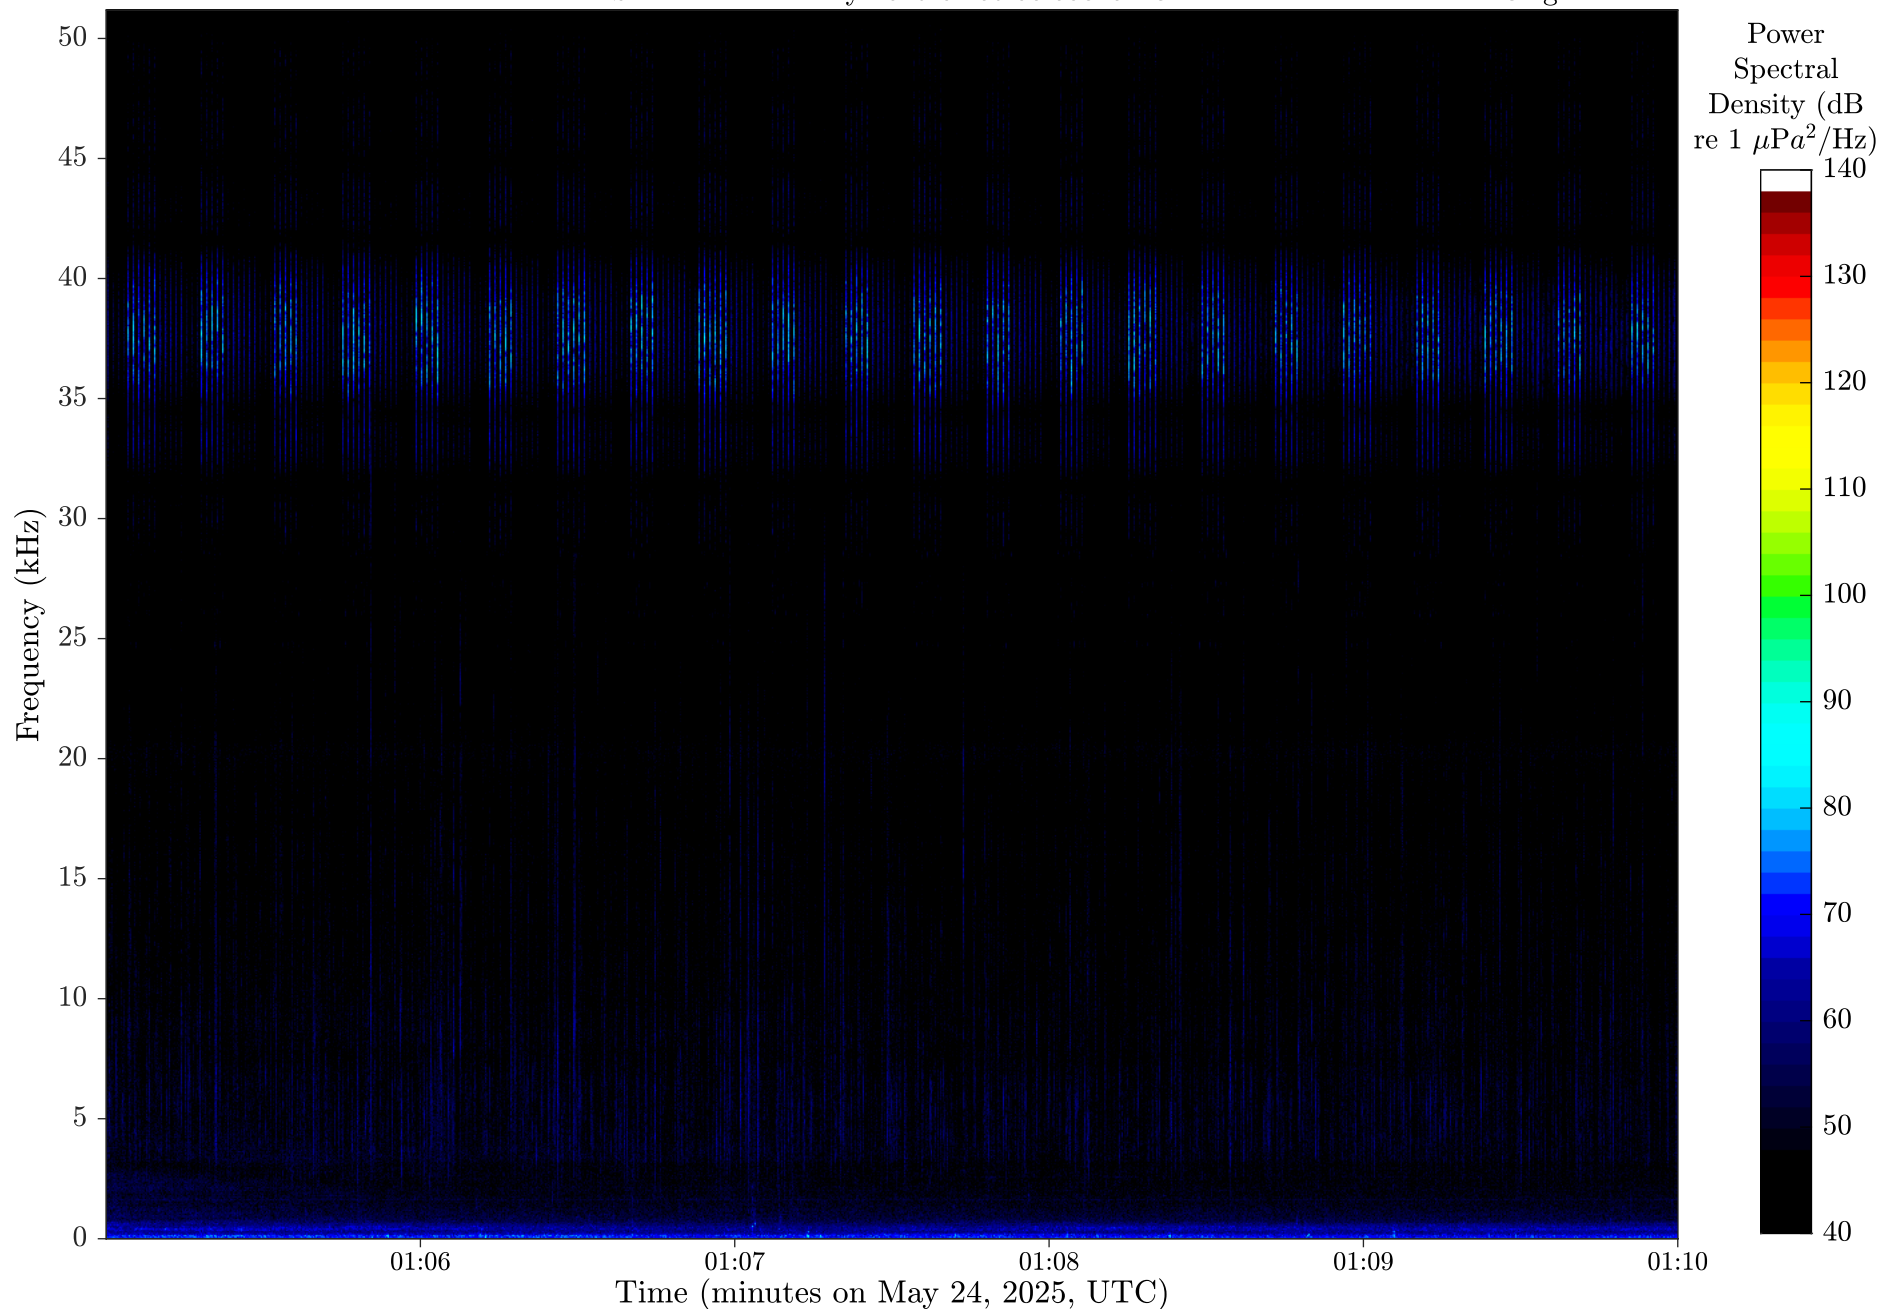

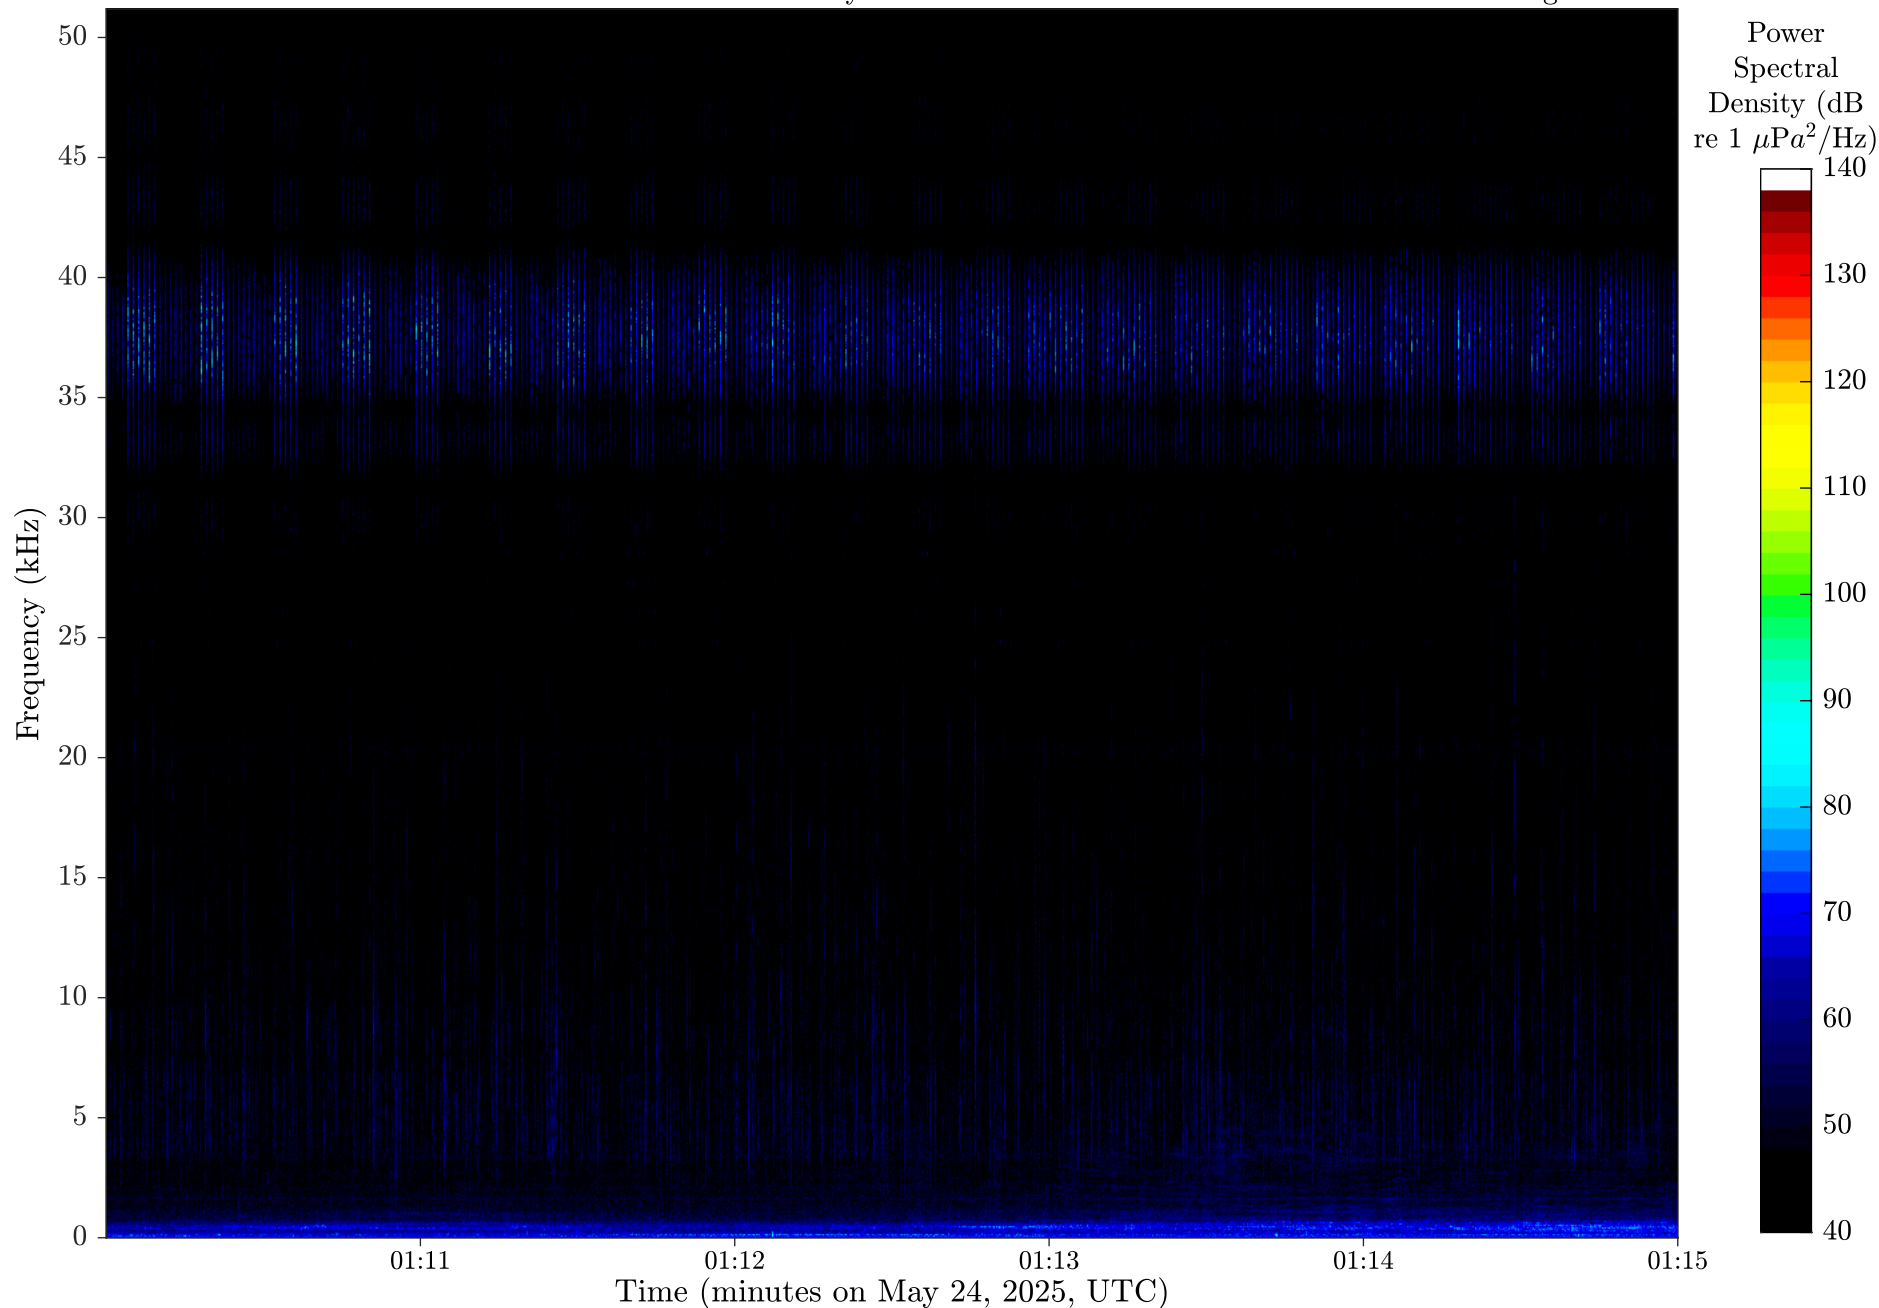


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:16:53 UTC

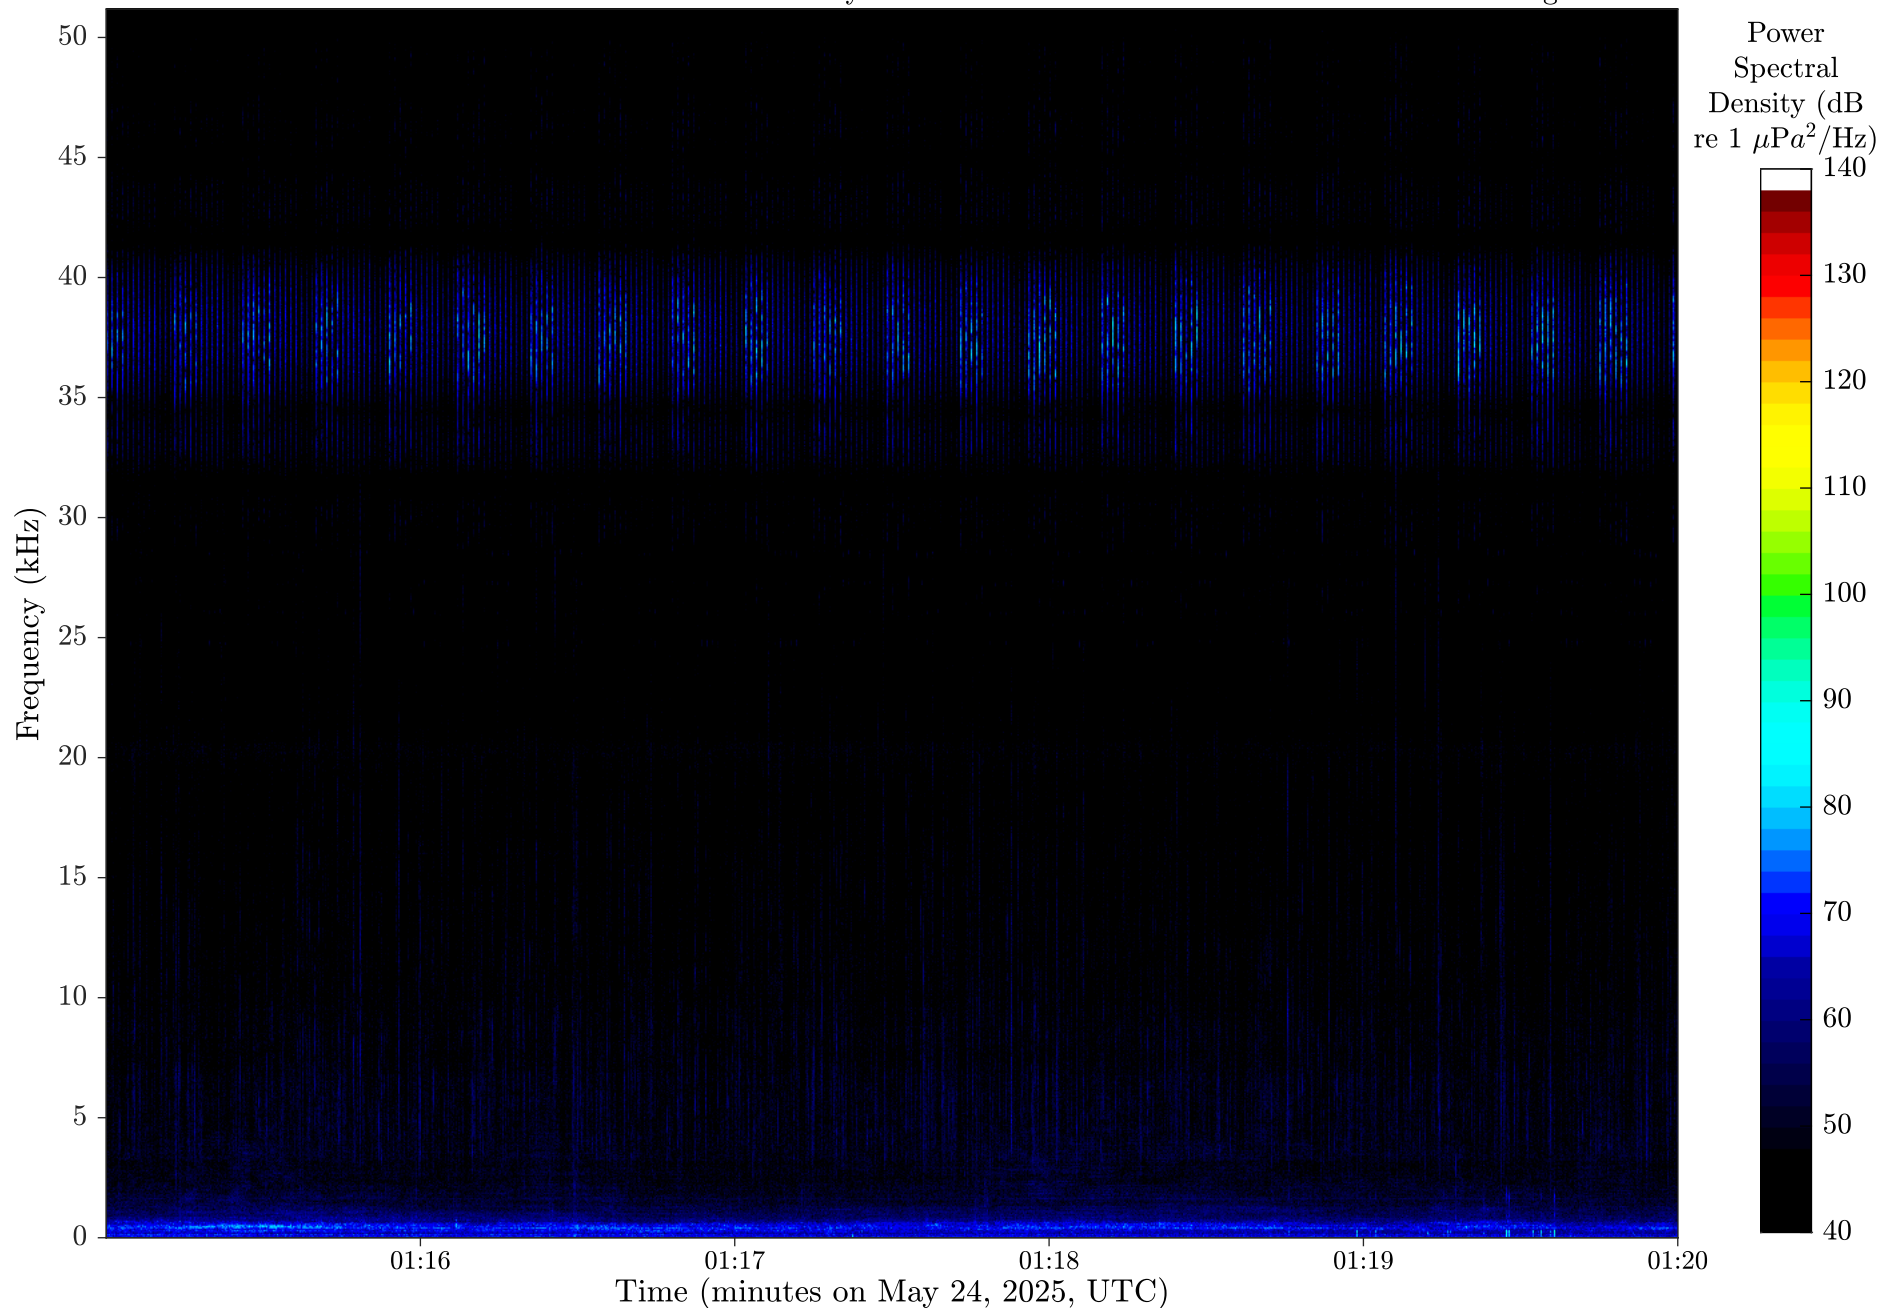


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:17:00 UTC

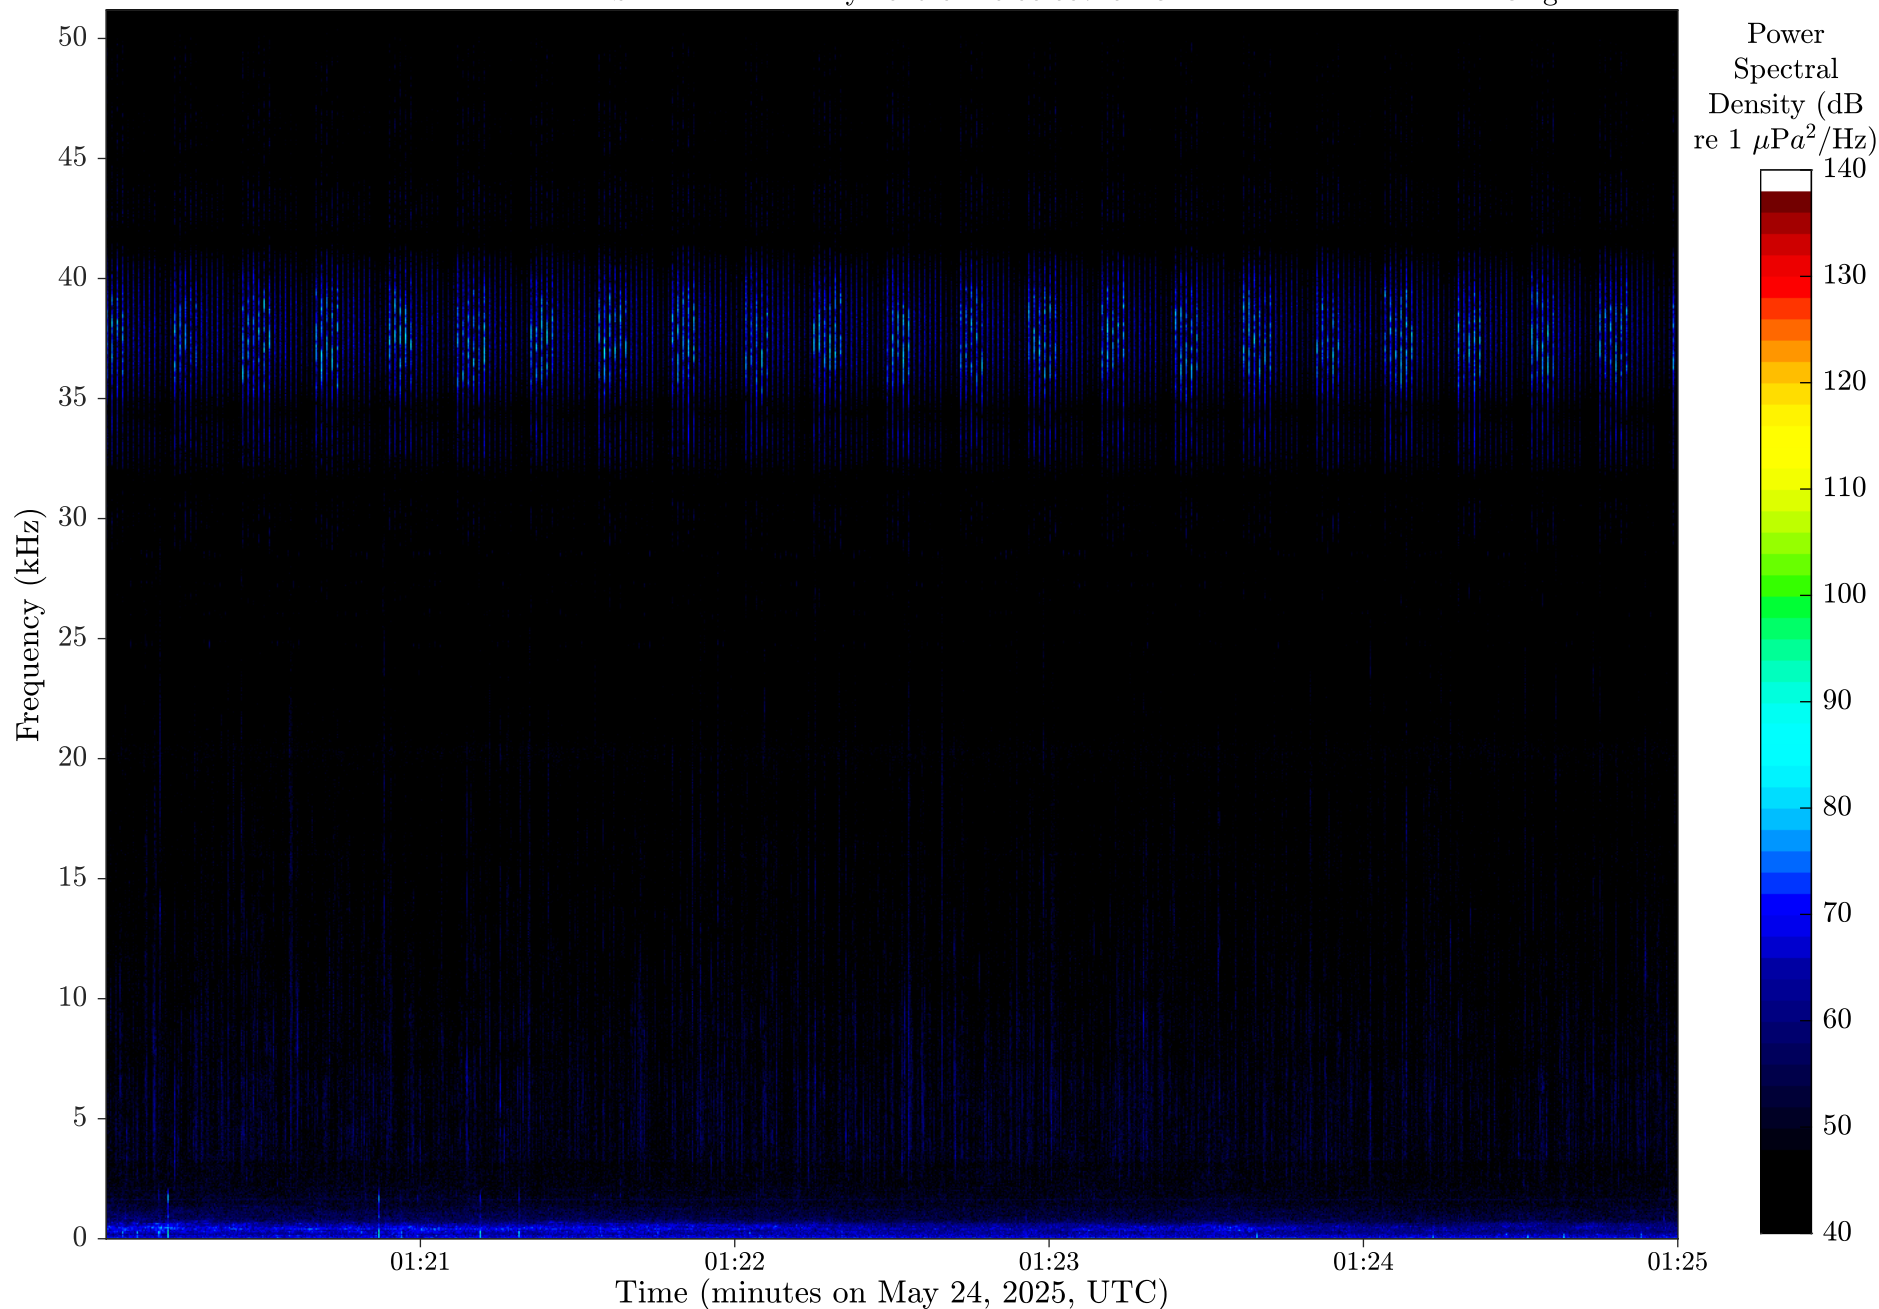


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:17:09 UTC

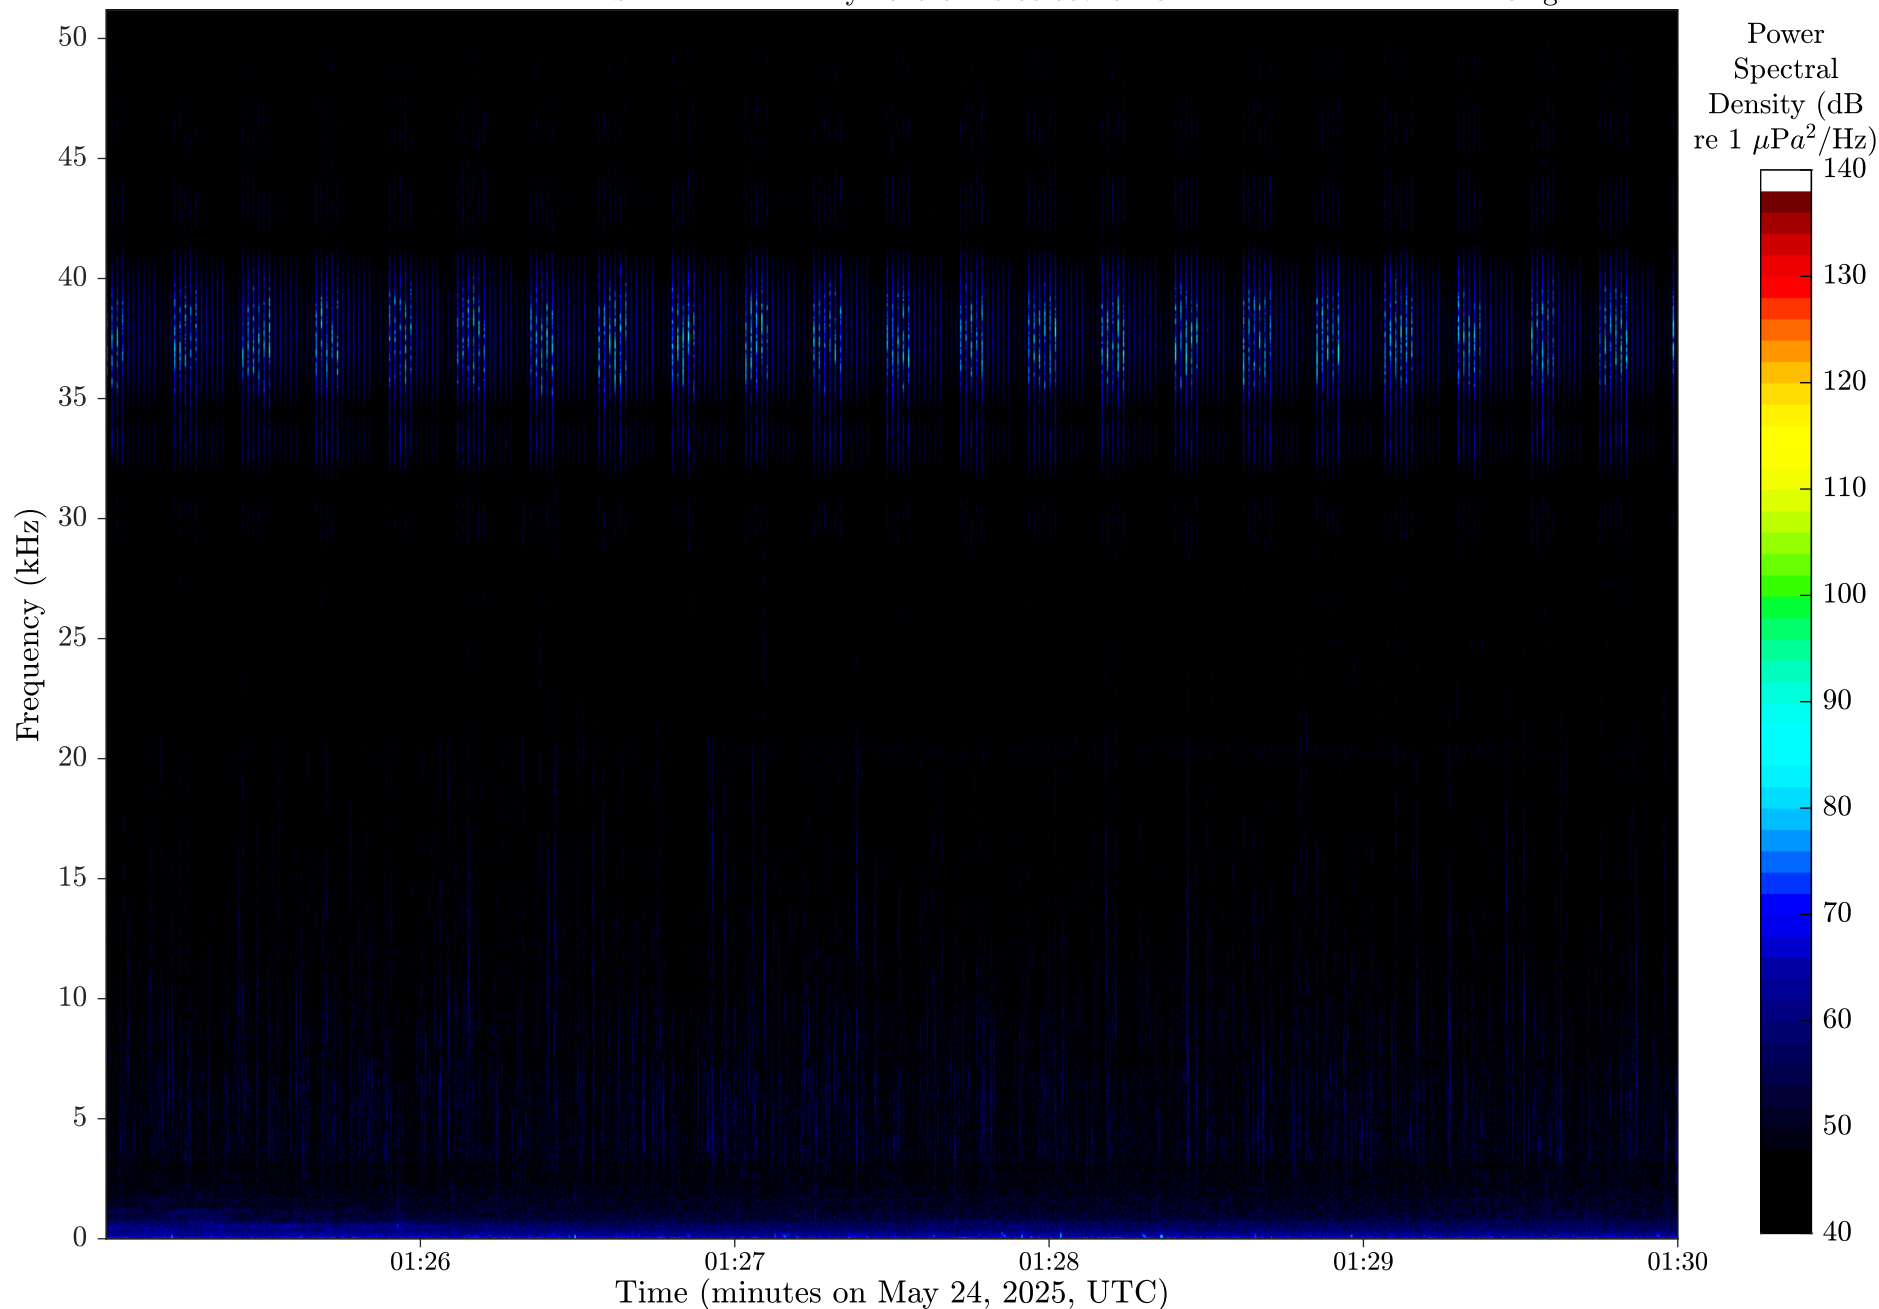

Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:17:18 UTC

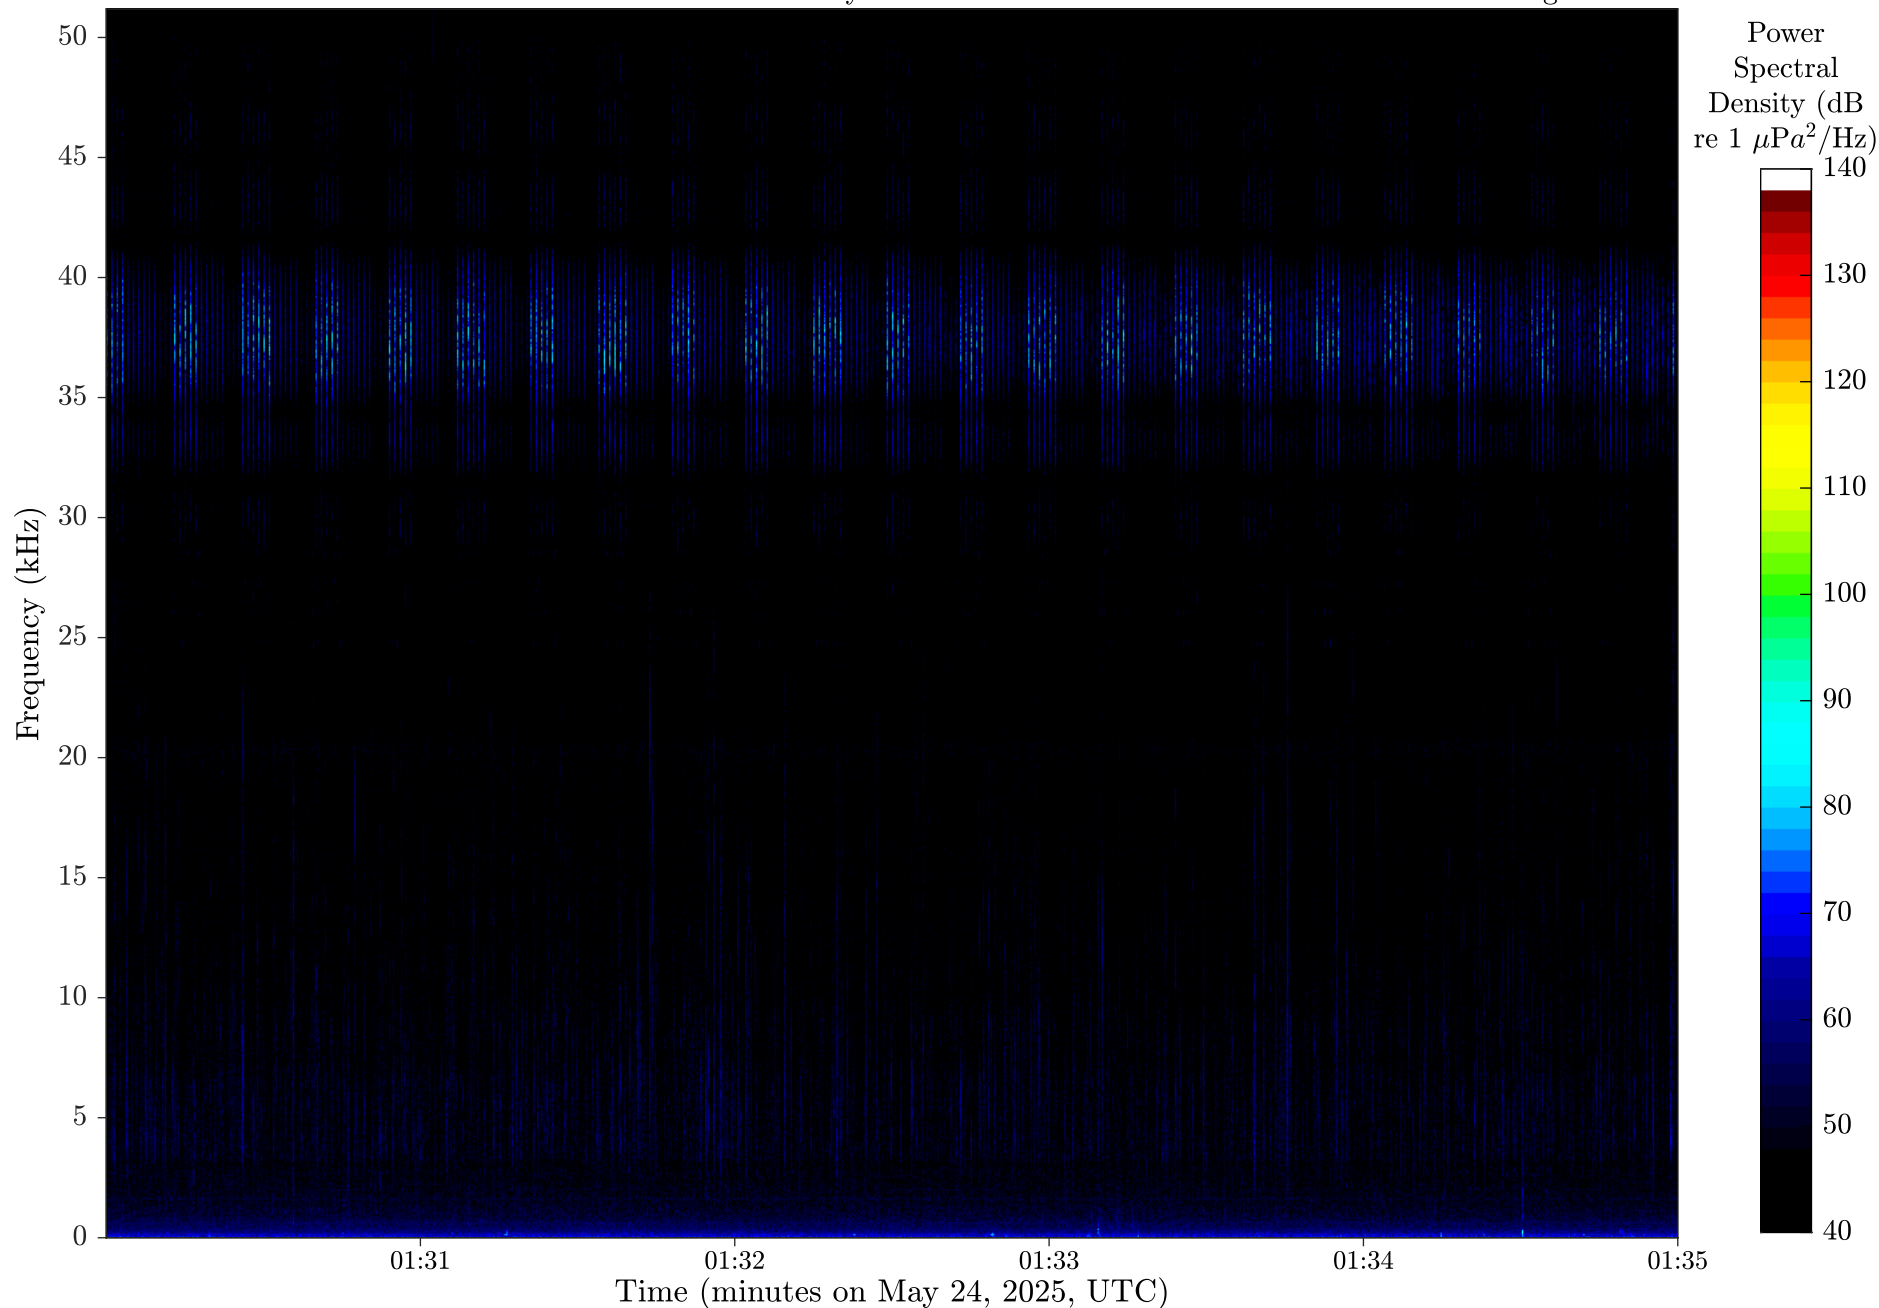

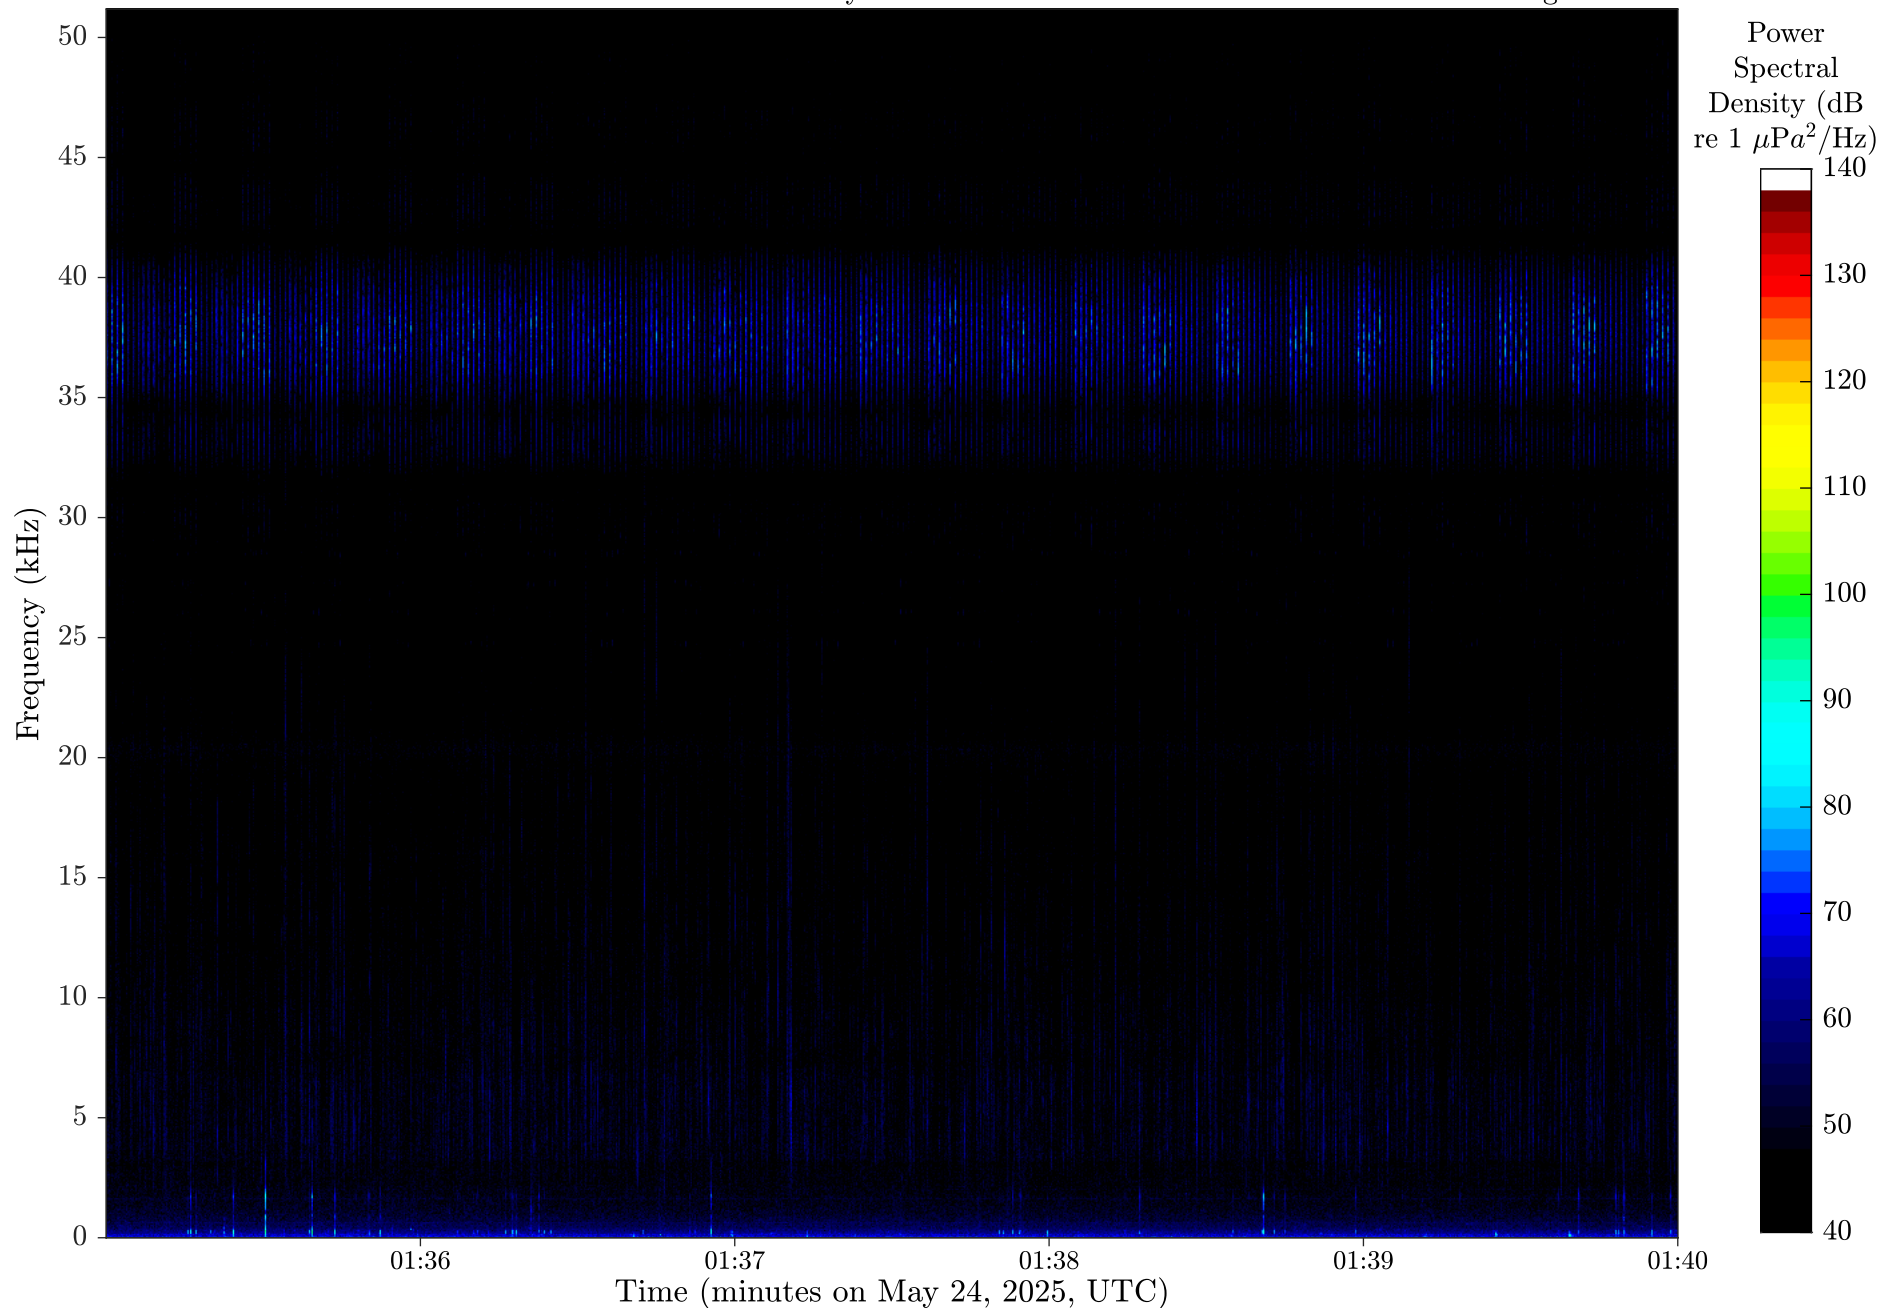


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:17:35 UTC

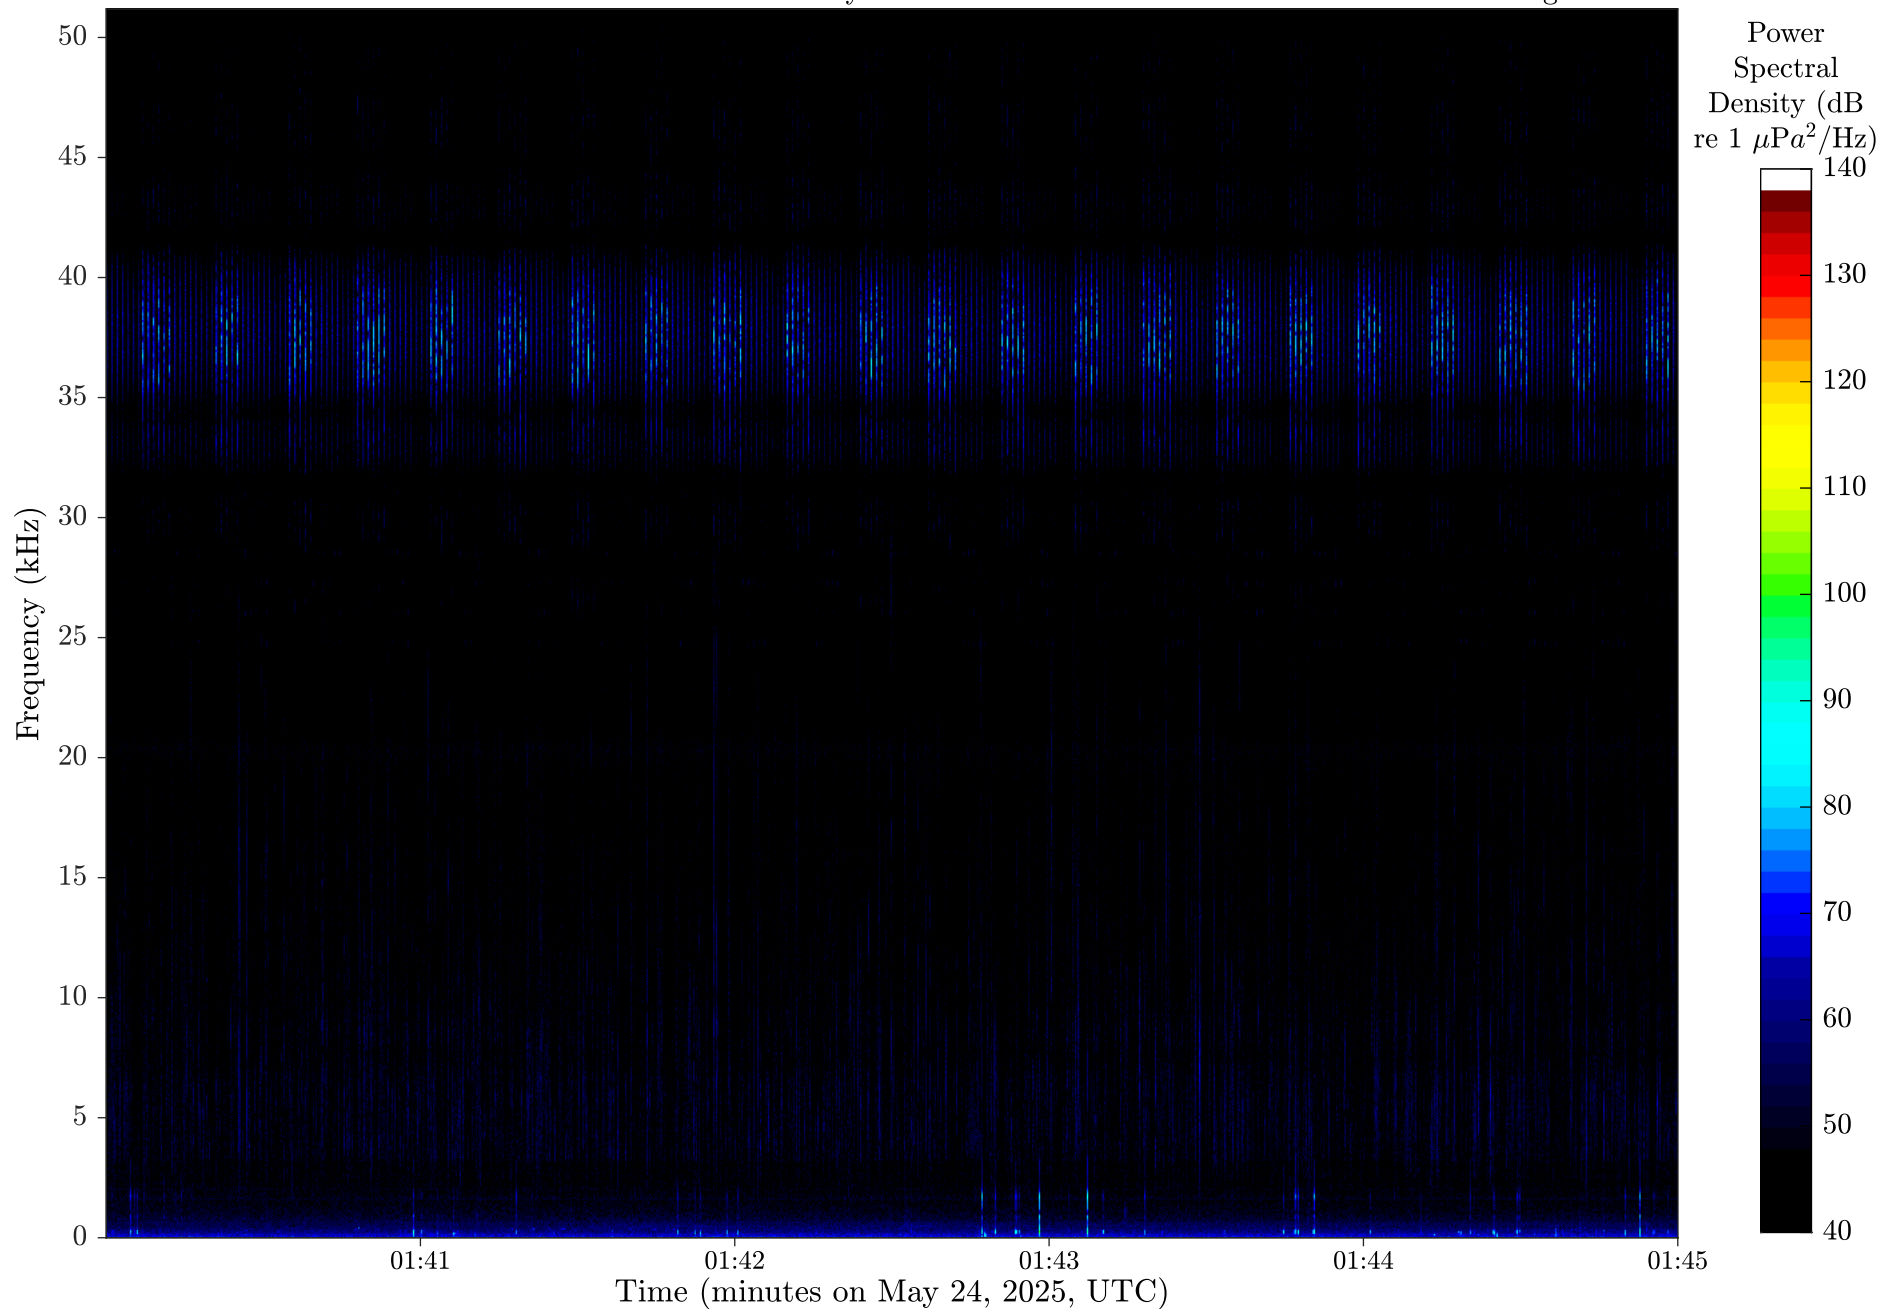


Comments: 34.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:17:43 UTC

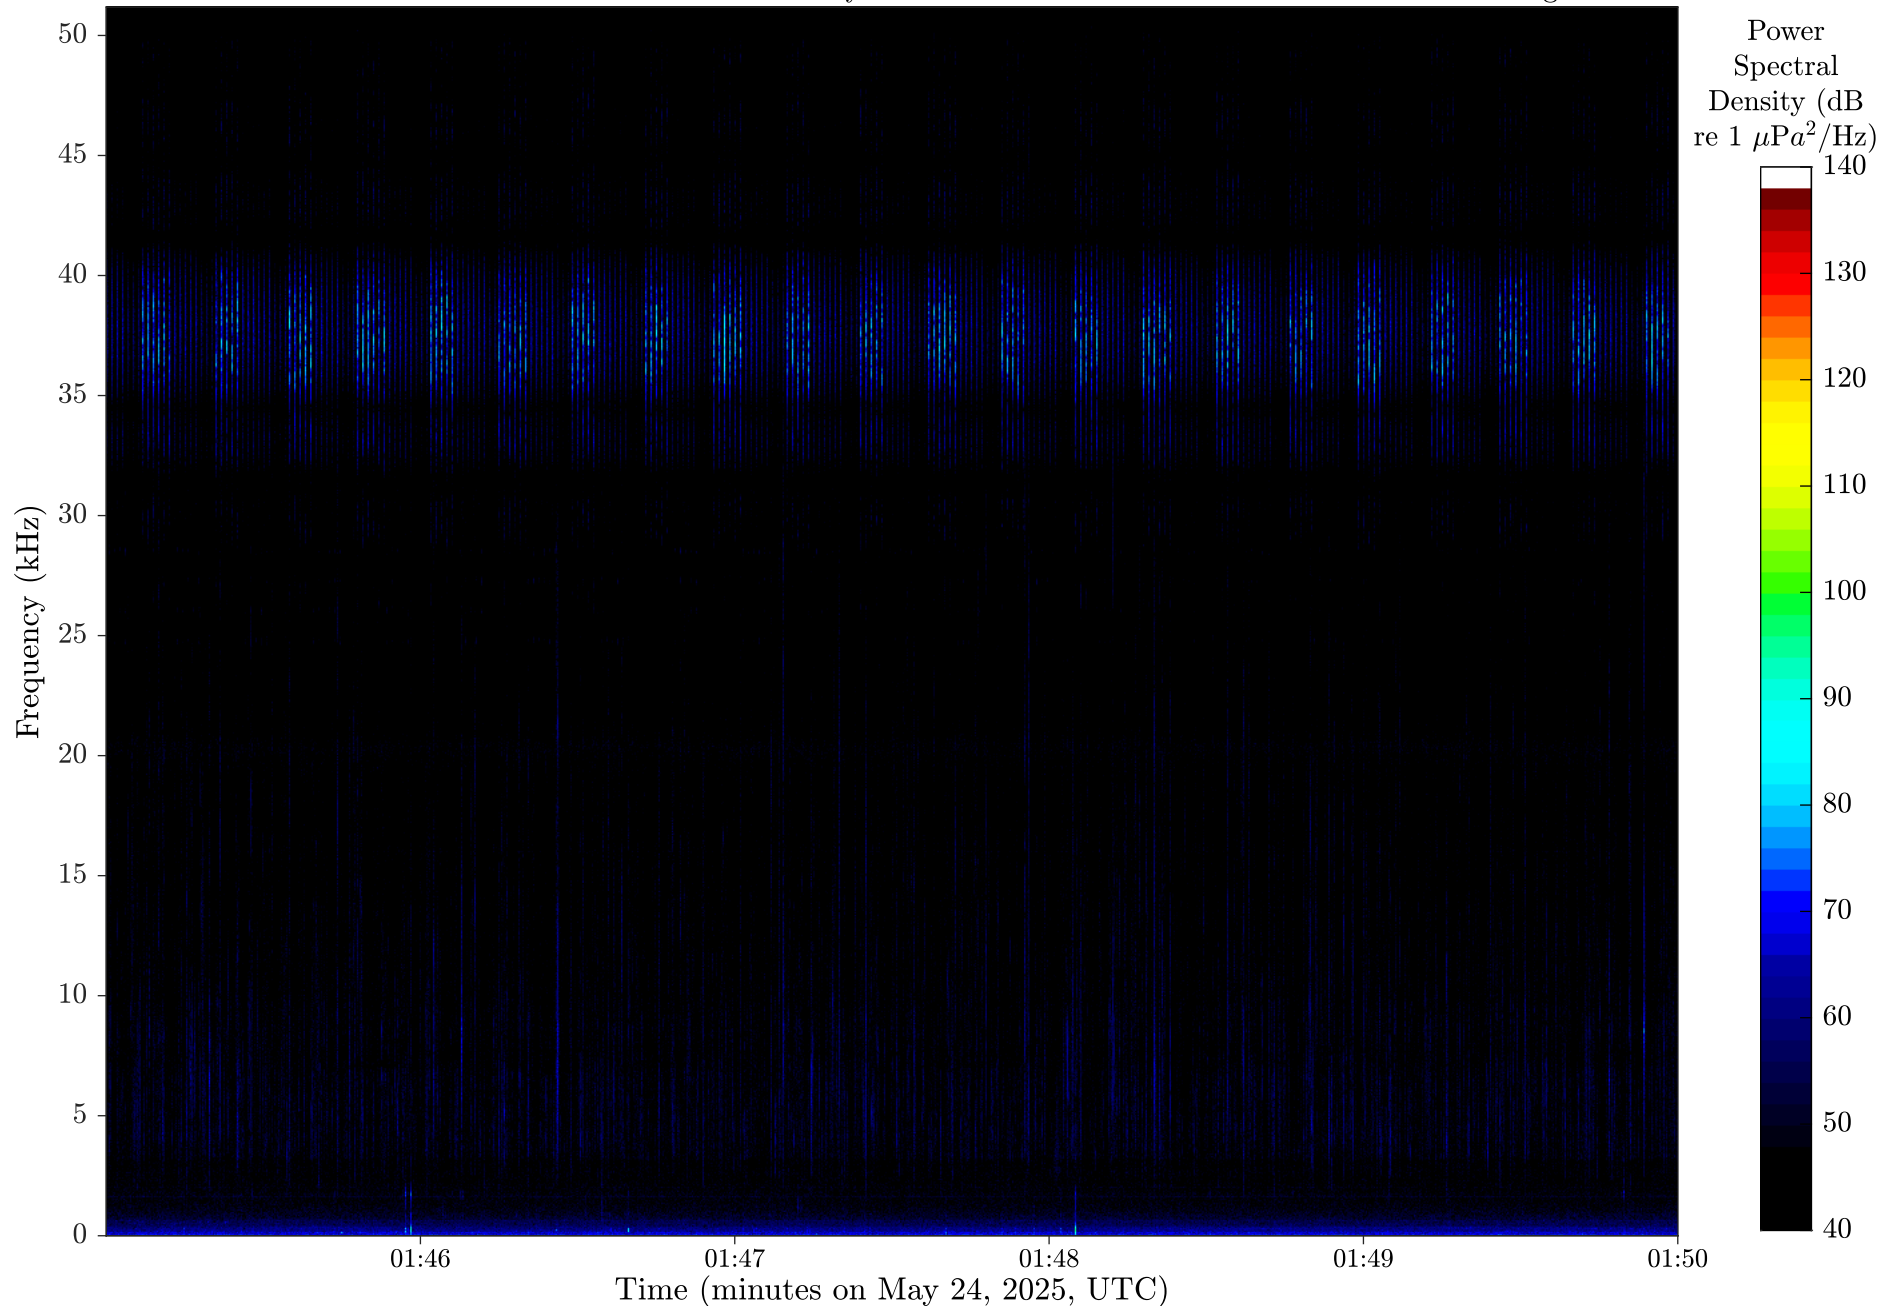


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:17:51 UTC

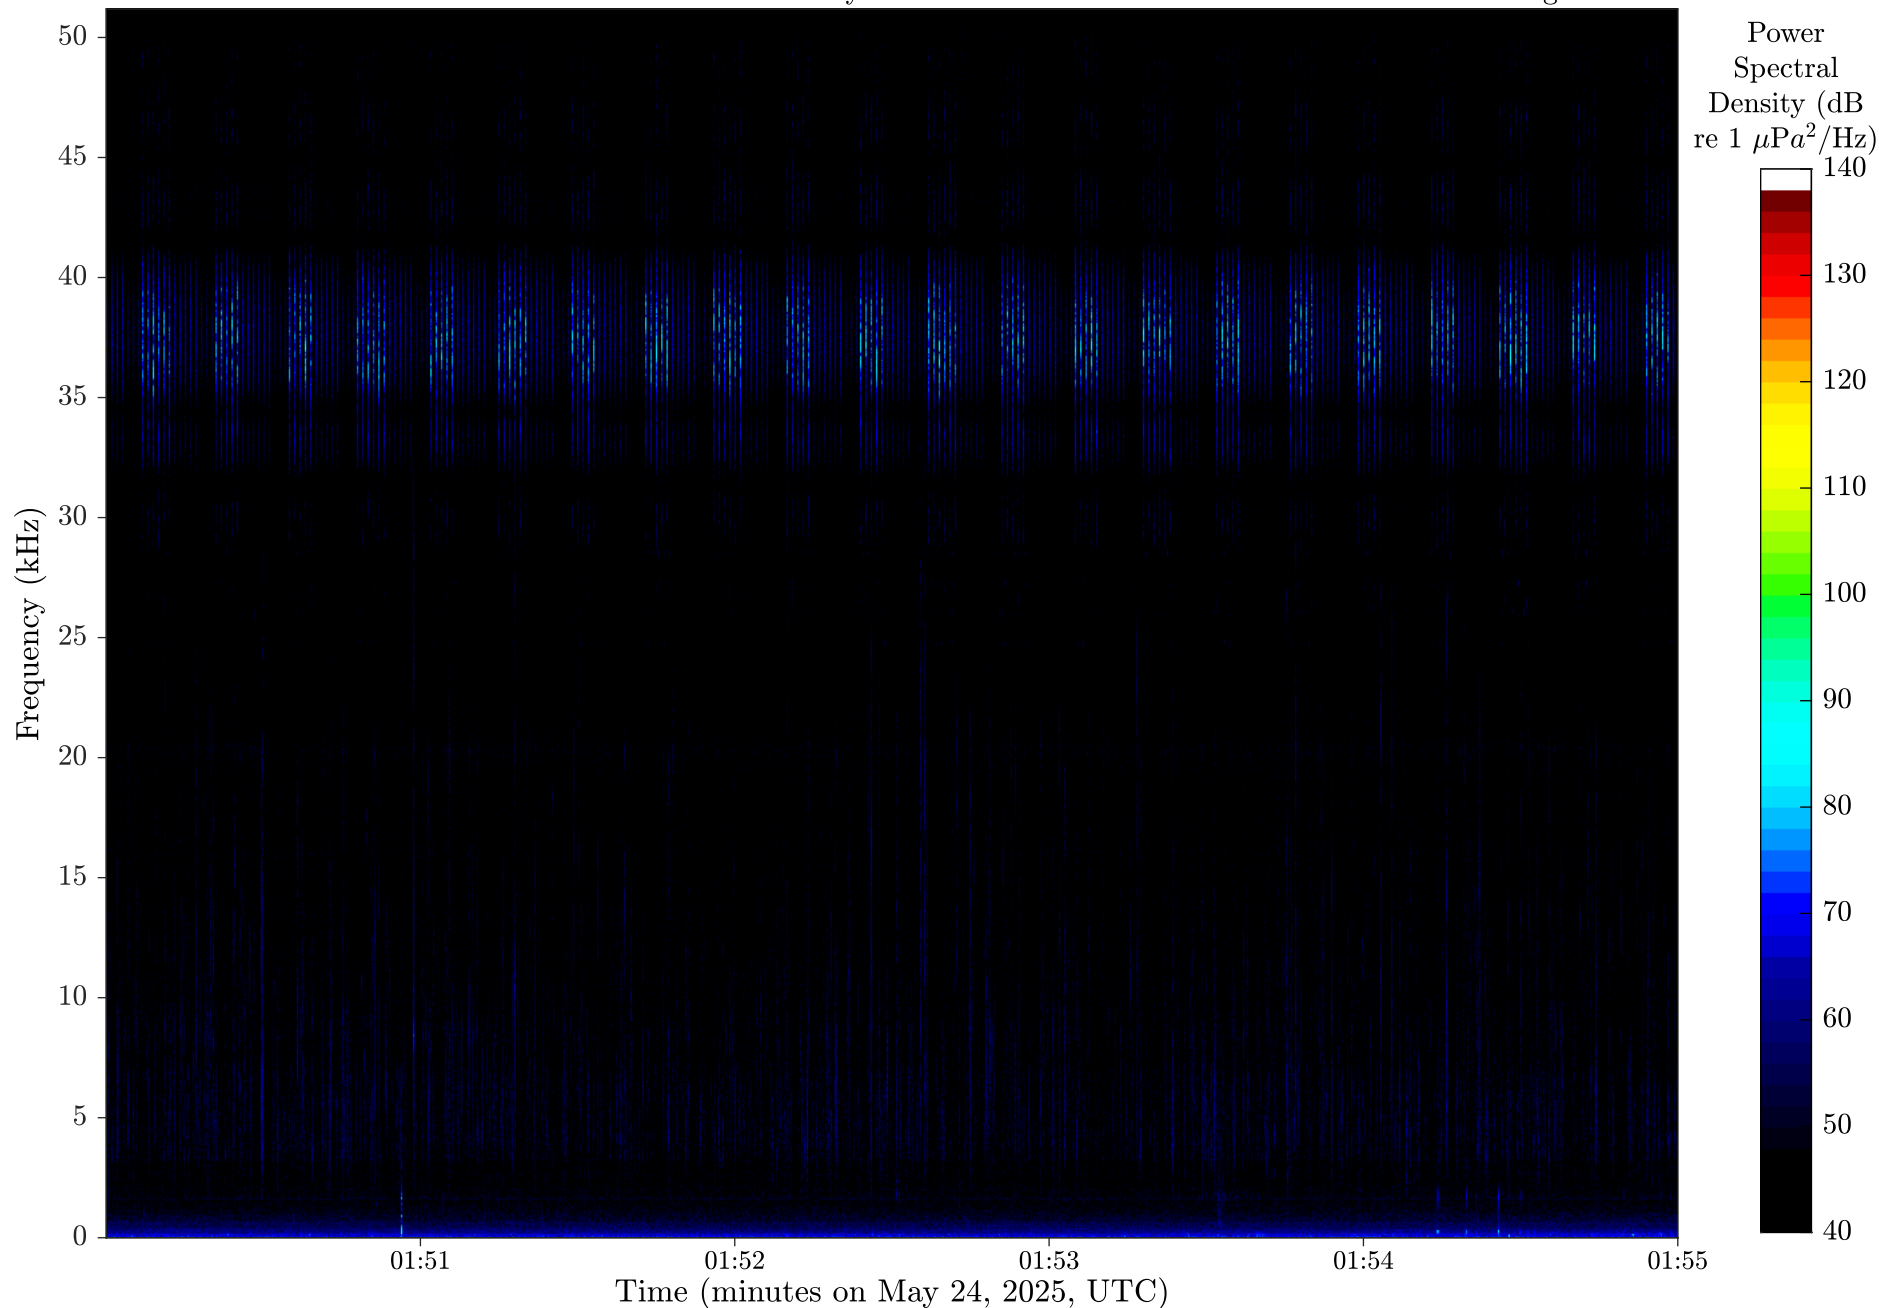


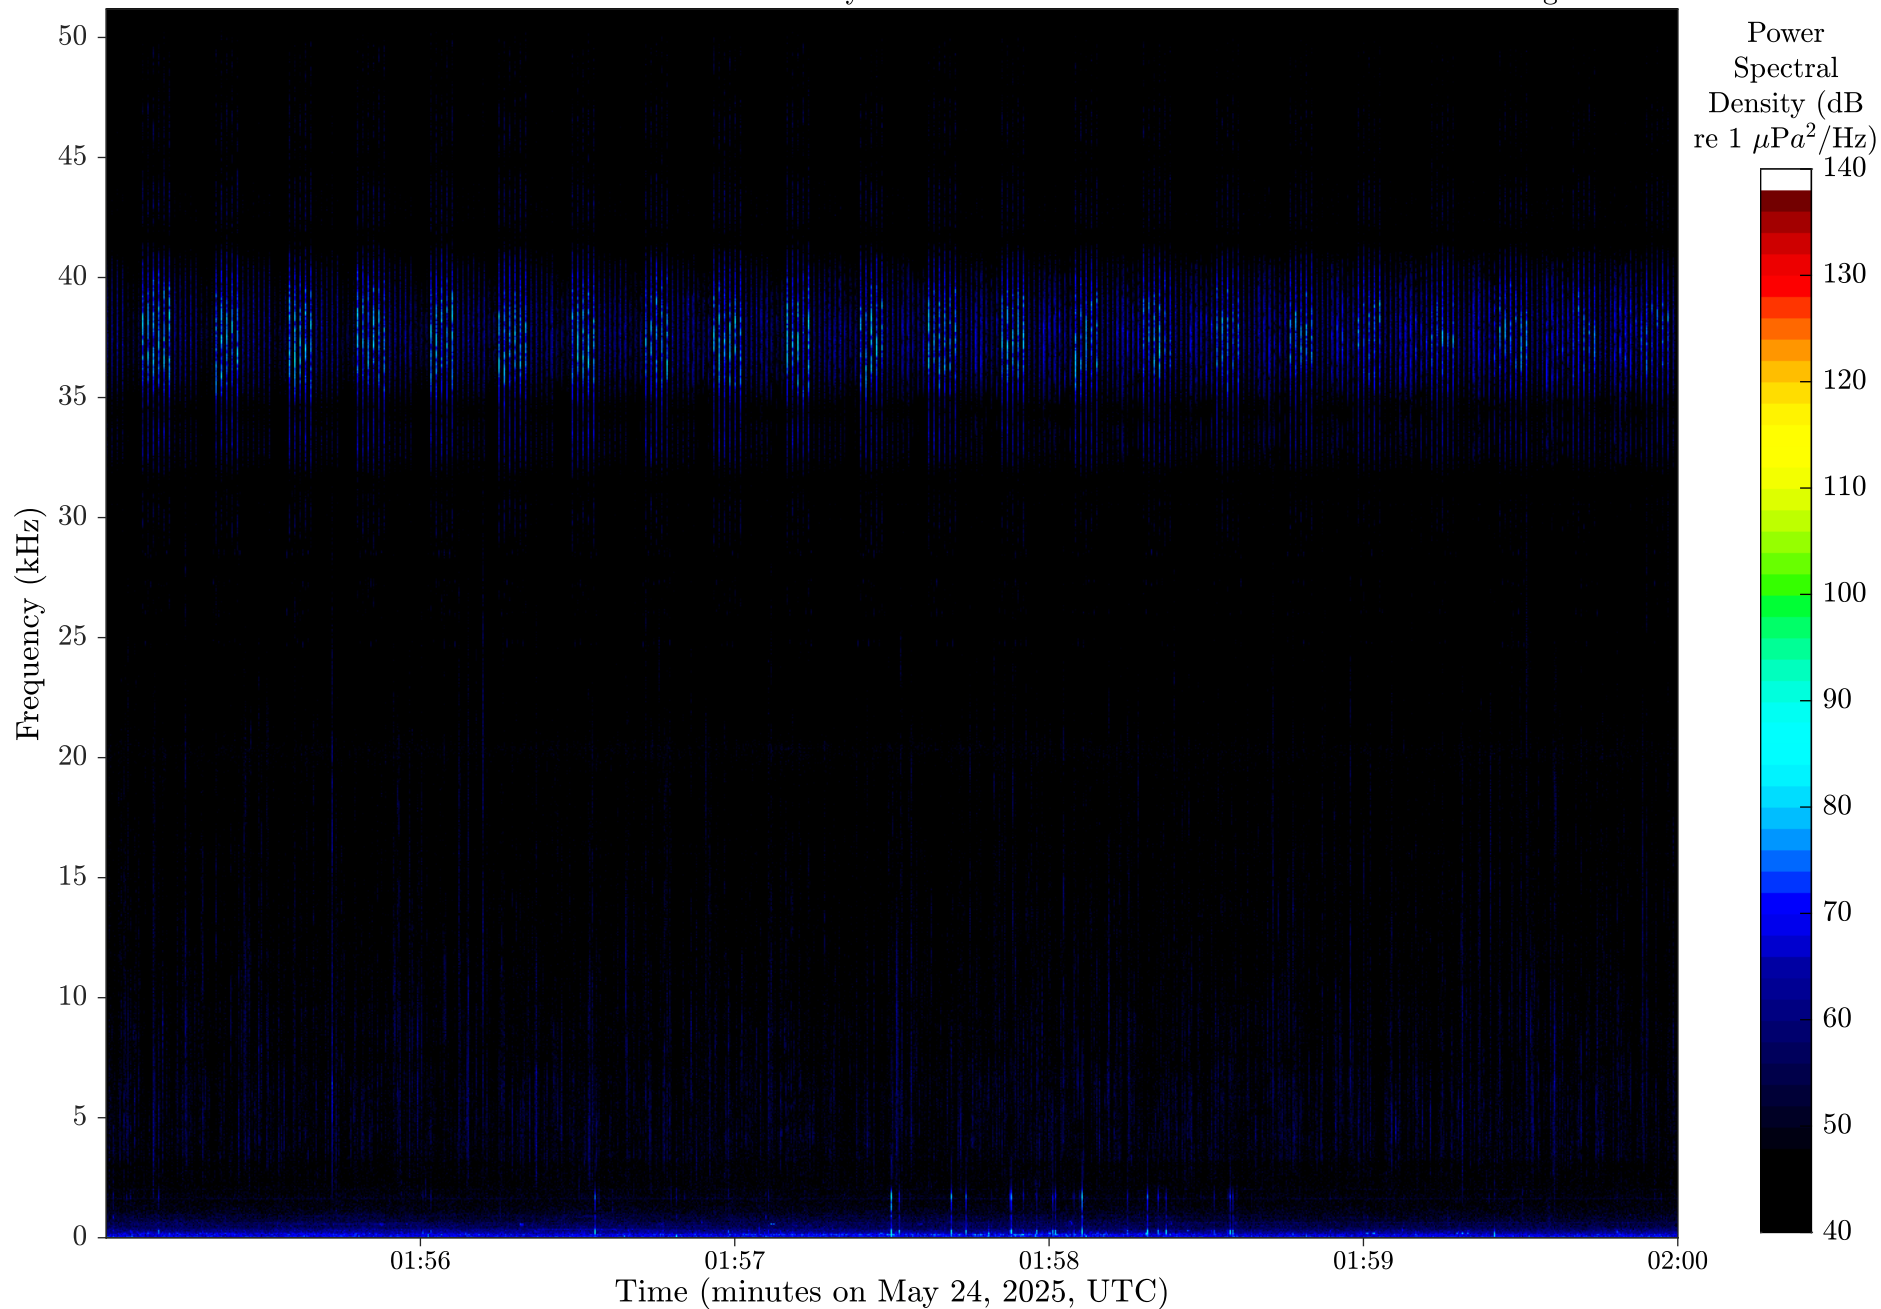

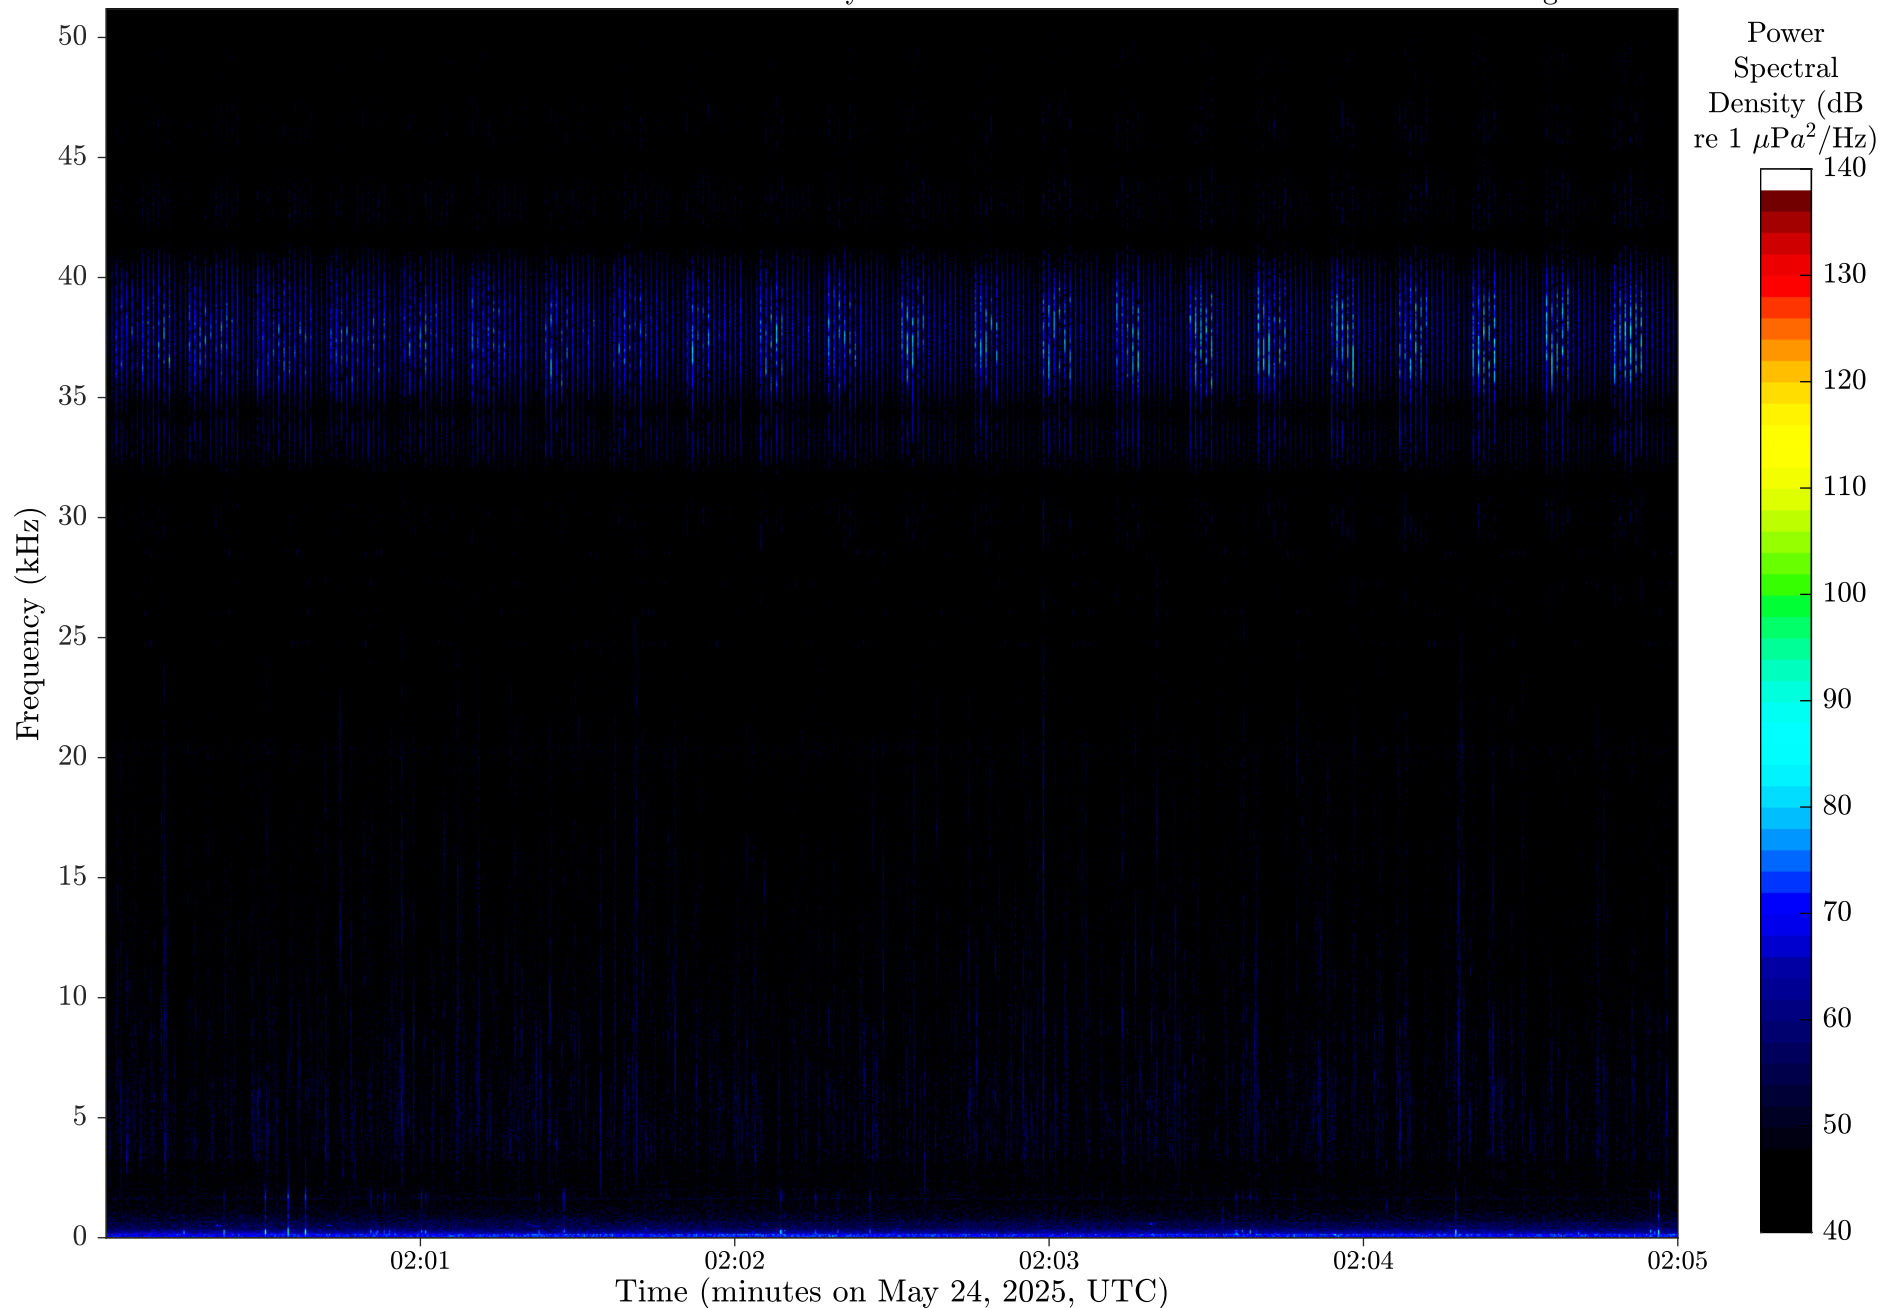


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:18:14 UTC

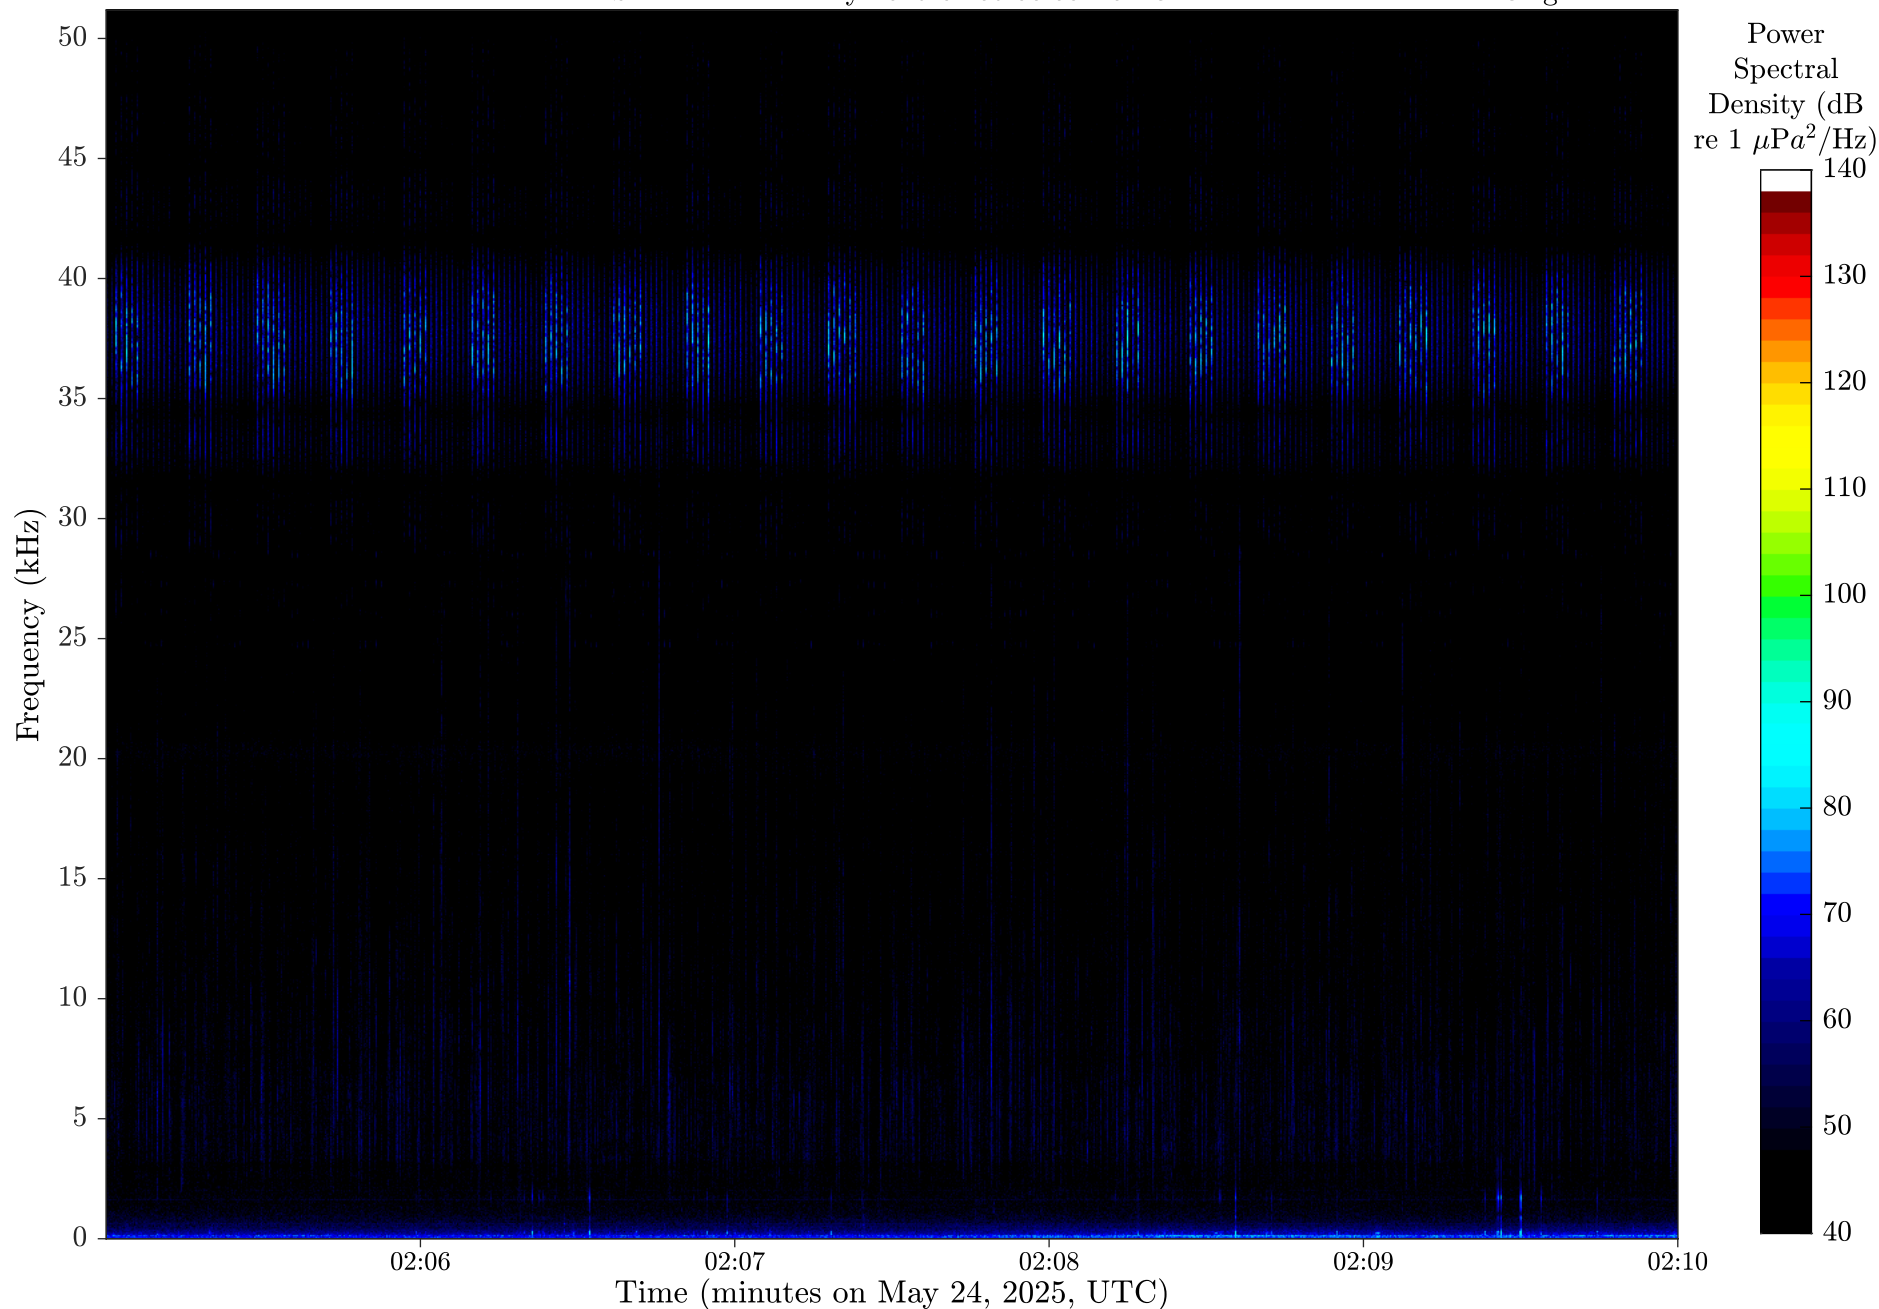


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:18:22 UTC

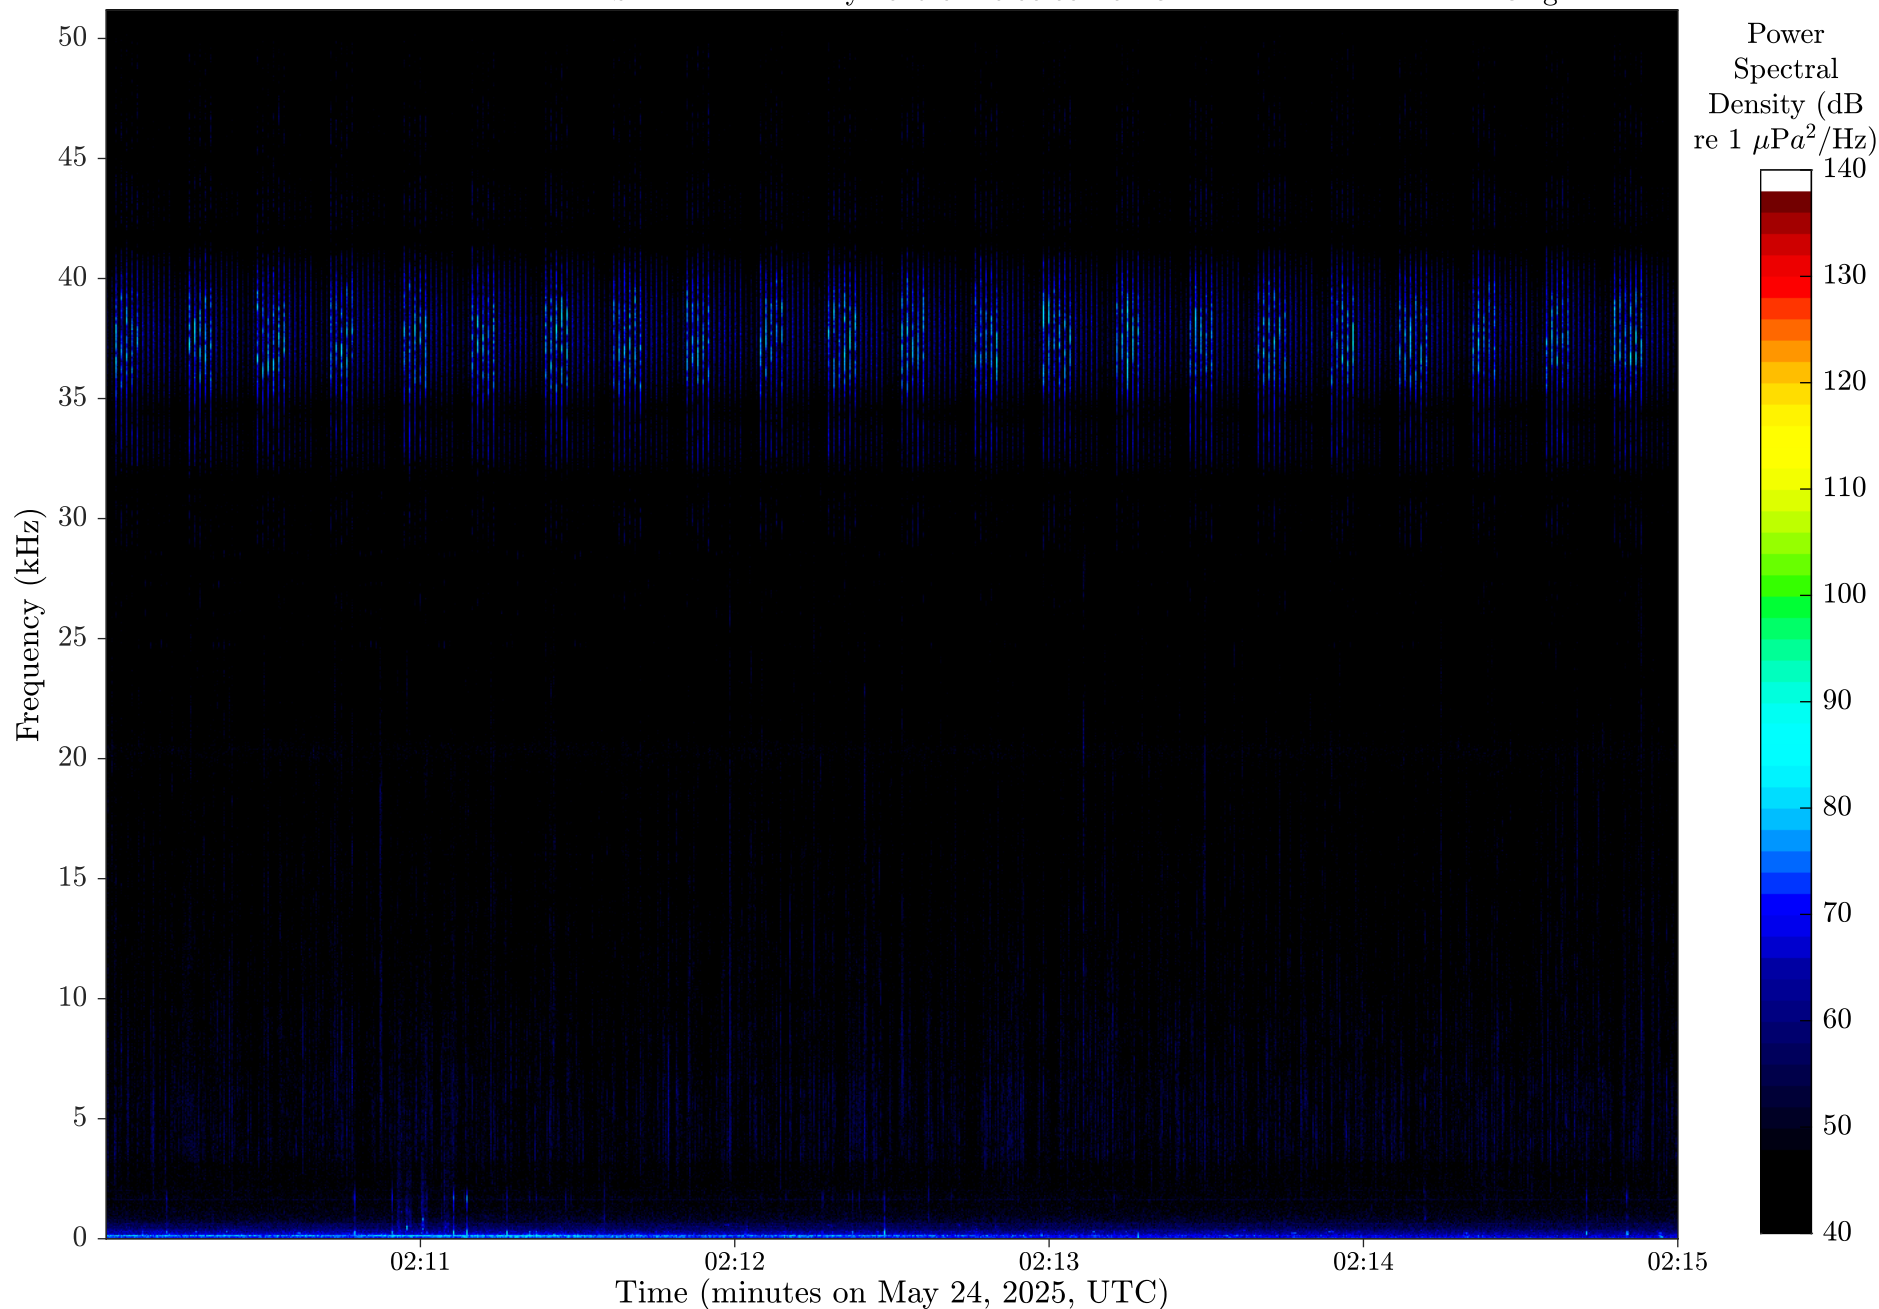

Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:18:31 UTC

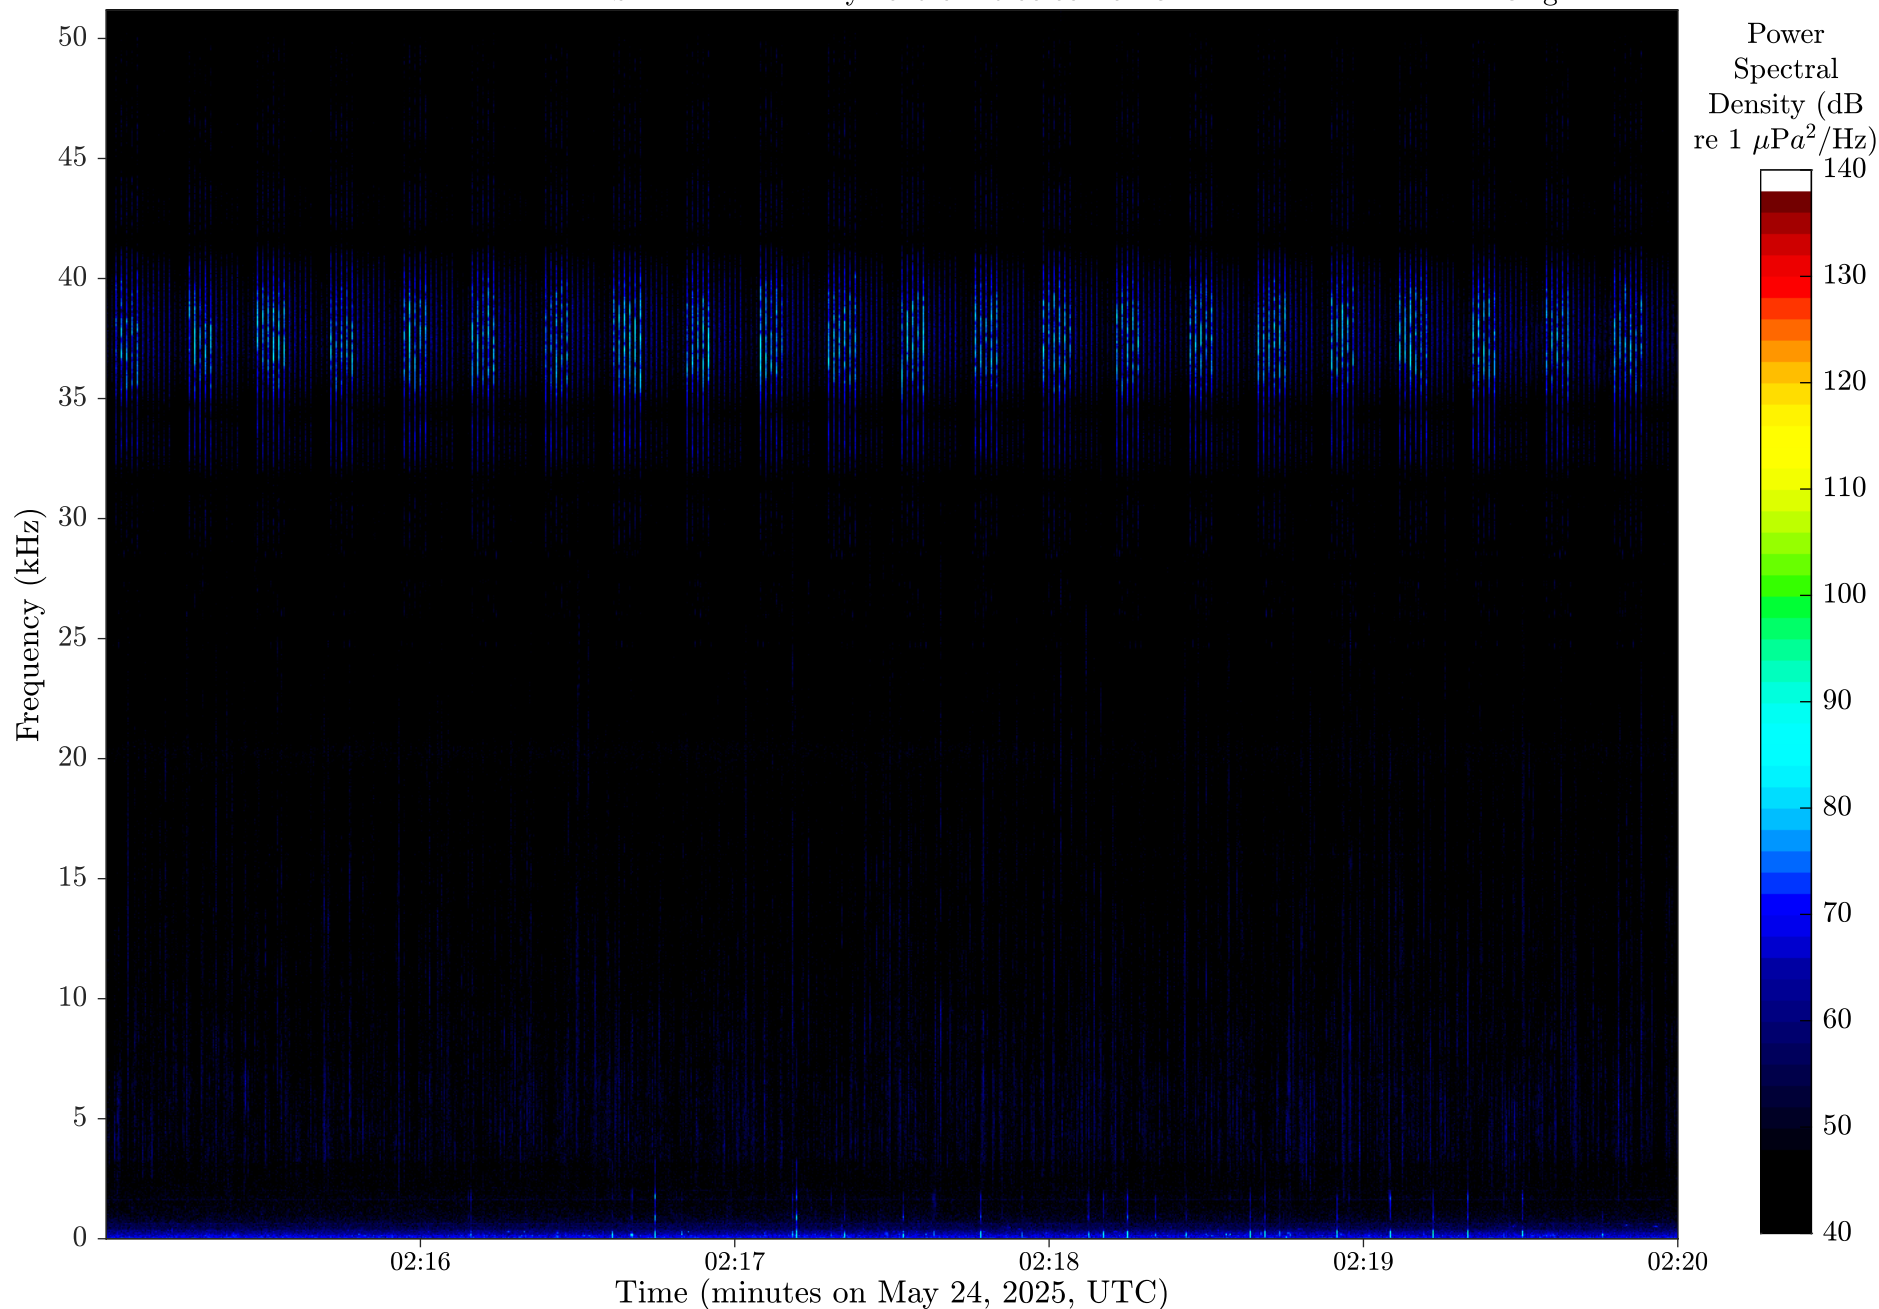

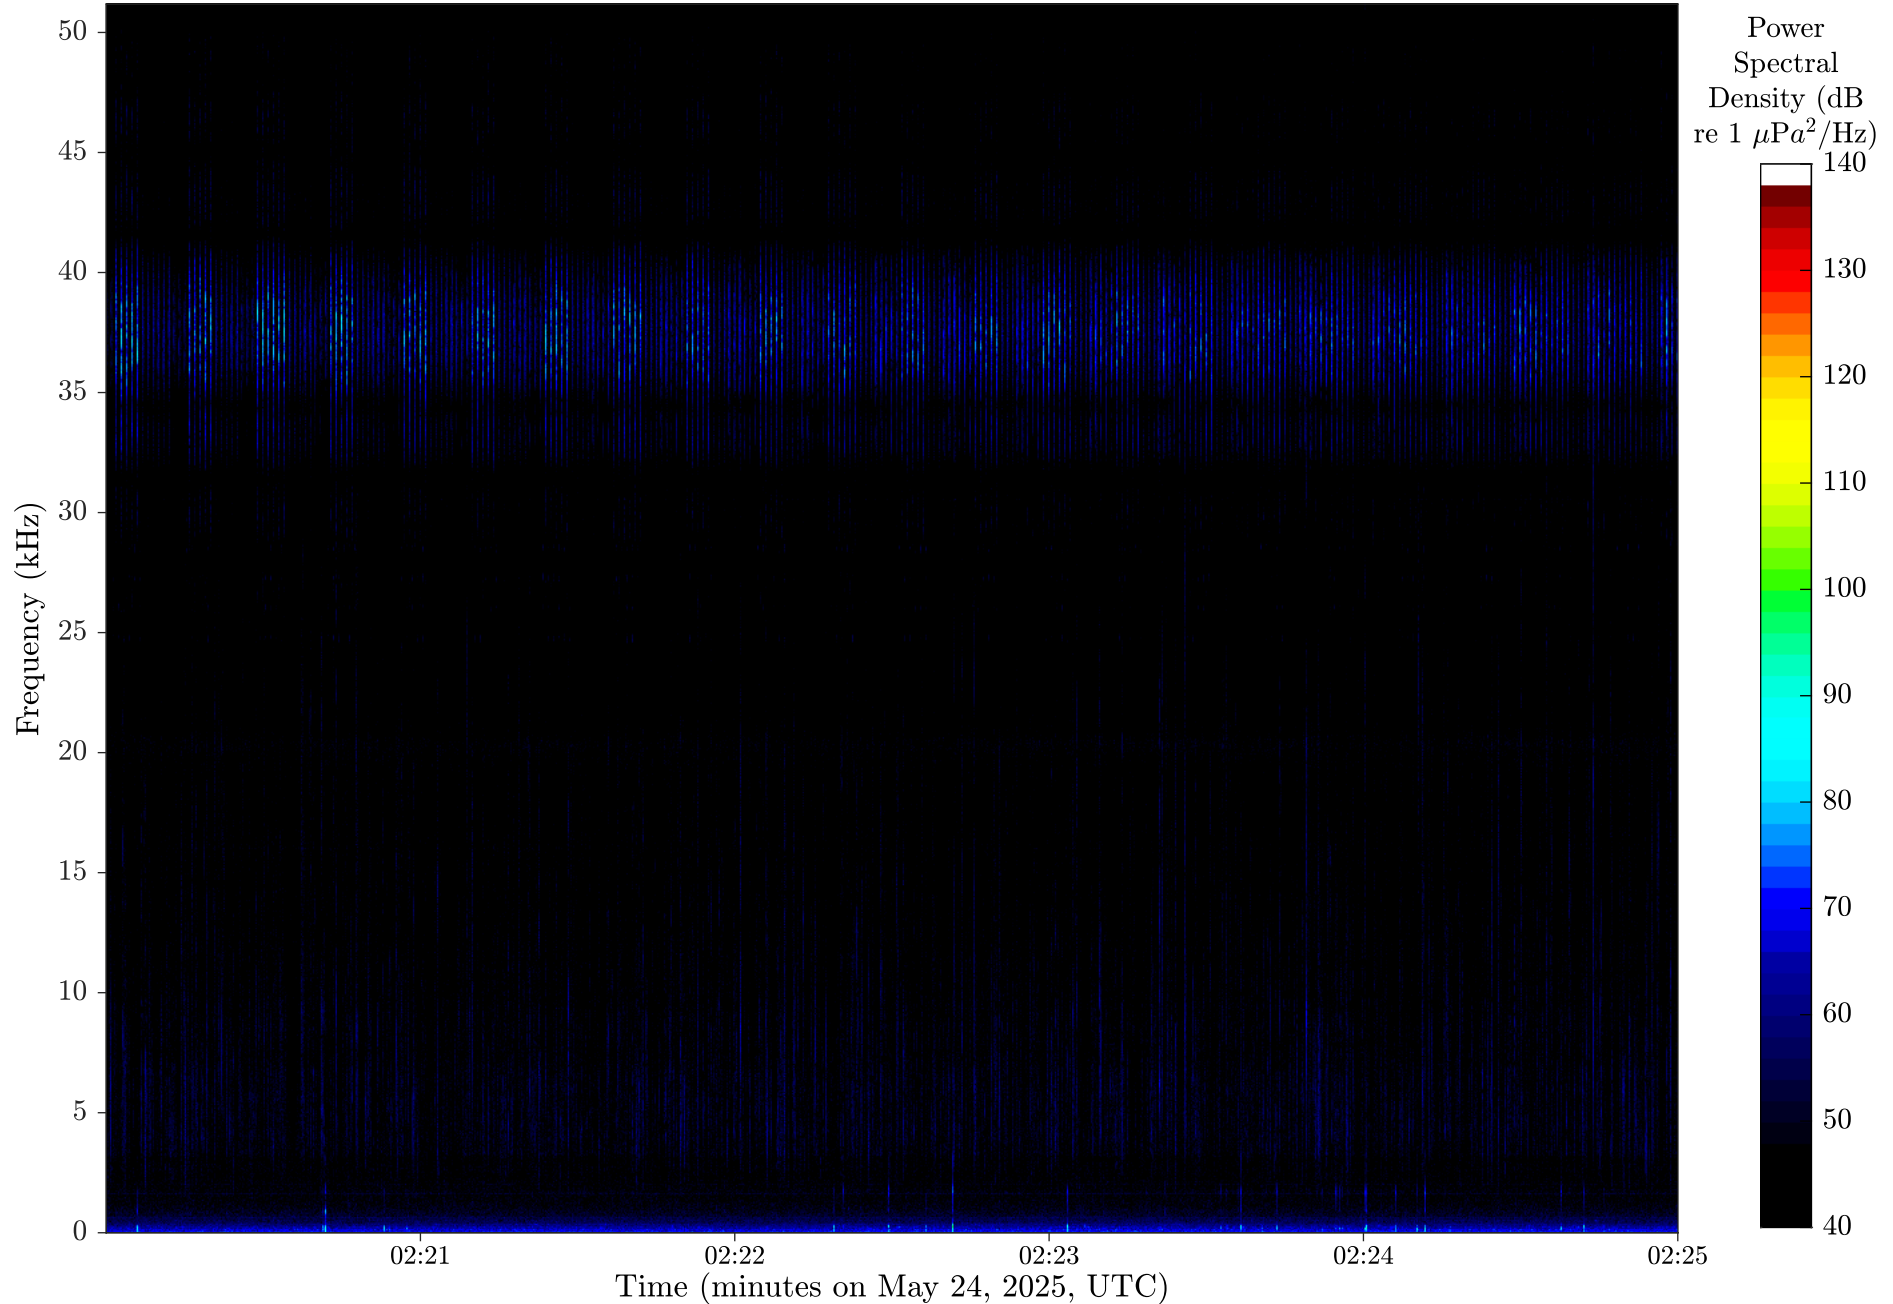


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:18:46 UTC

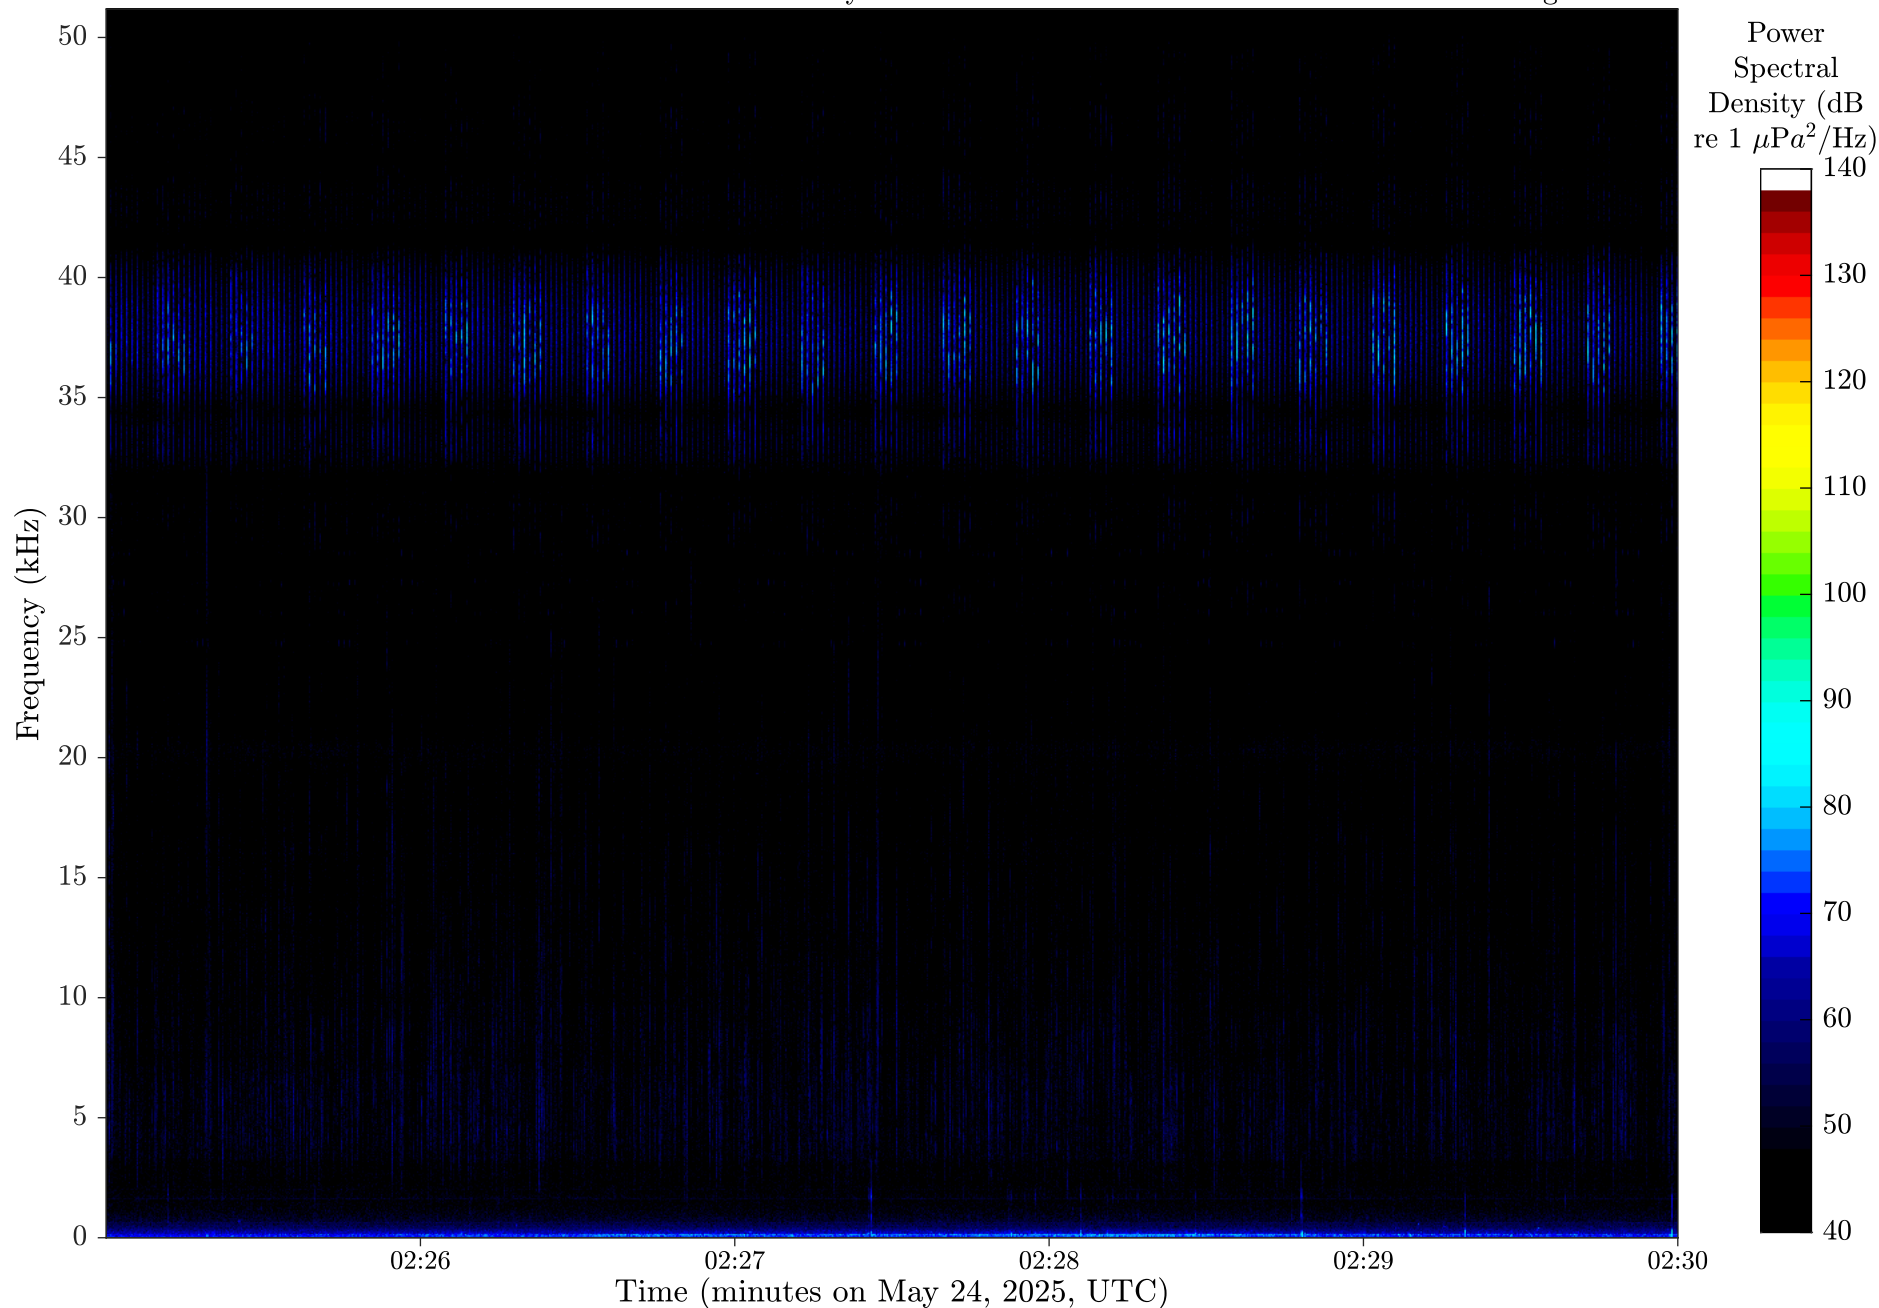


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:18:54 UTC

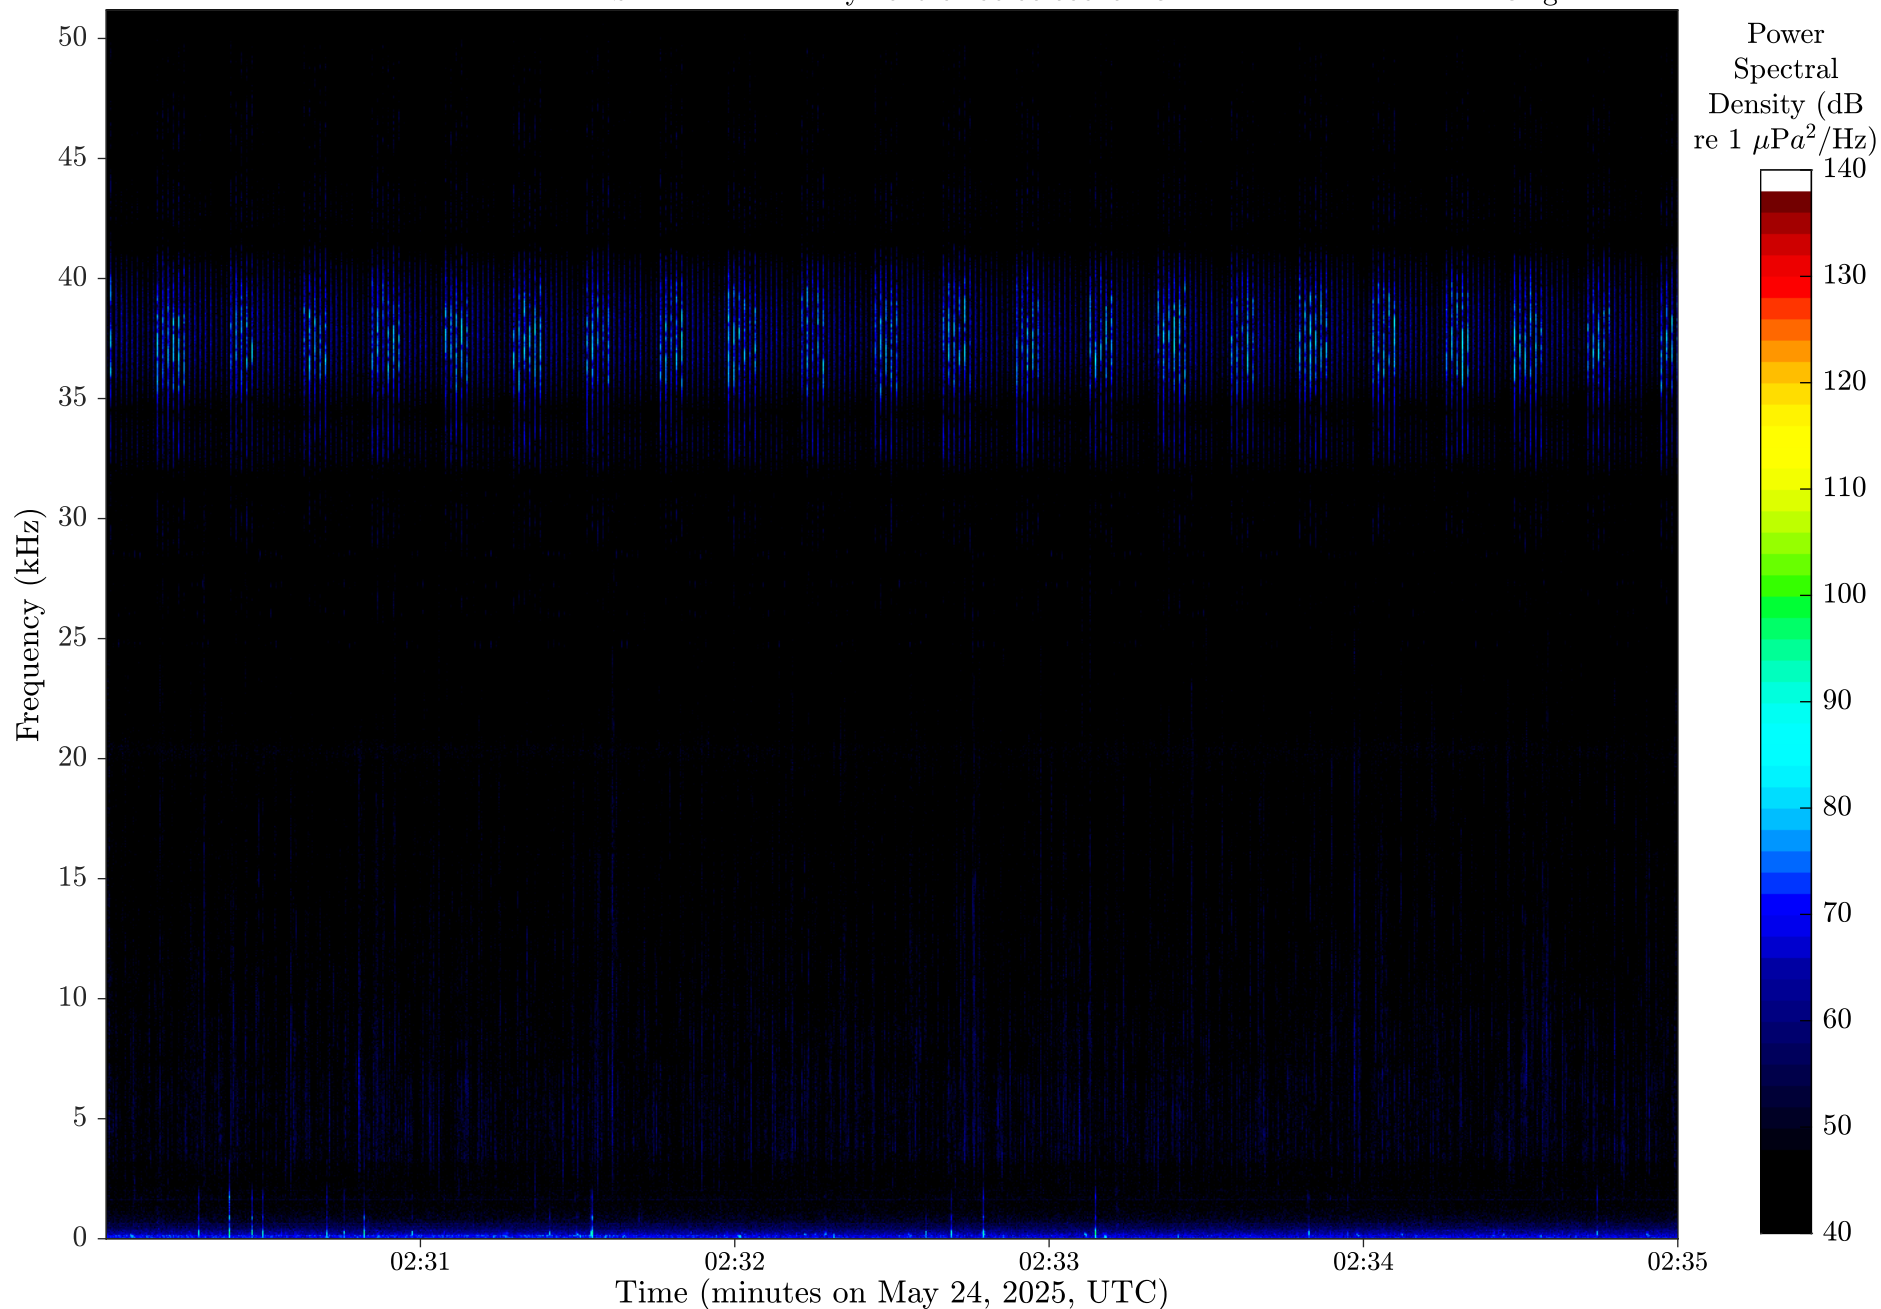


Comments: 35.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:19:02 UTC

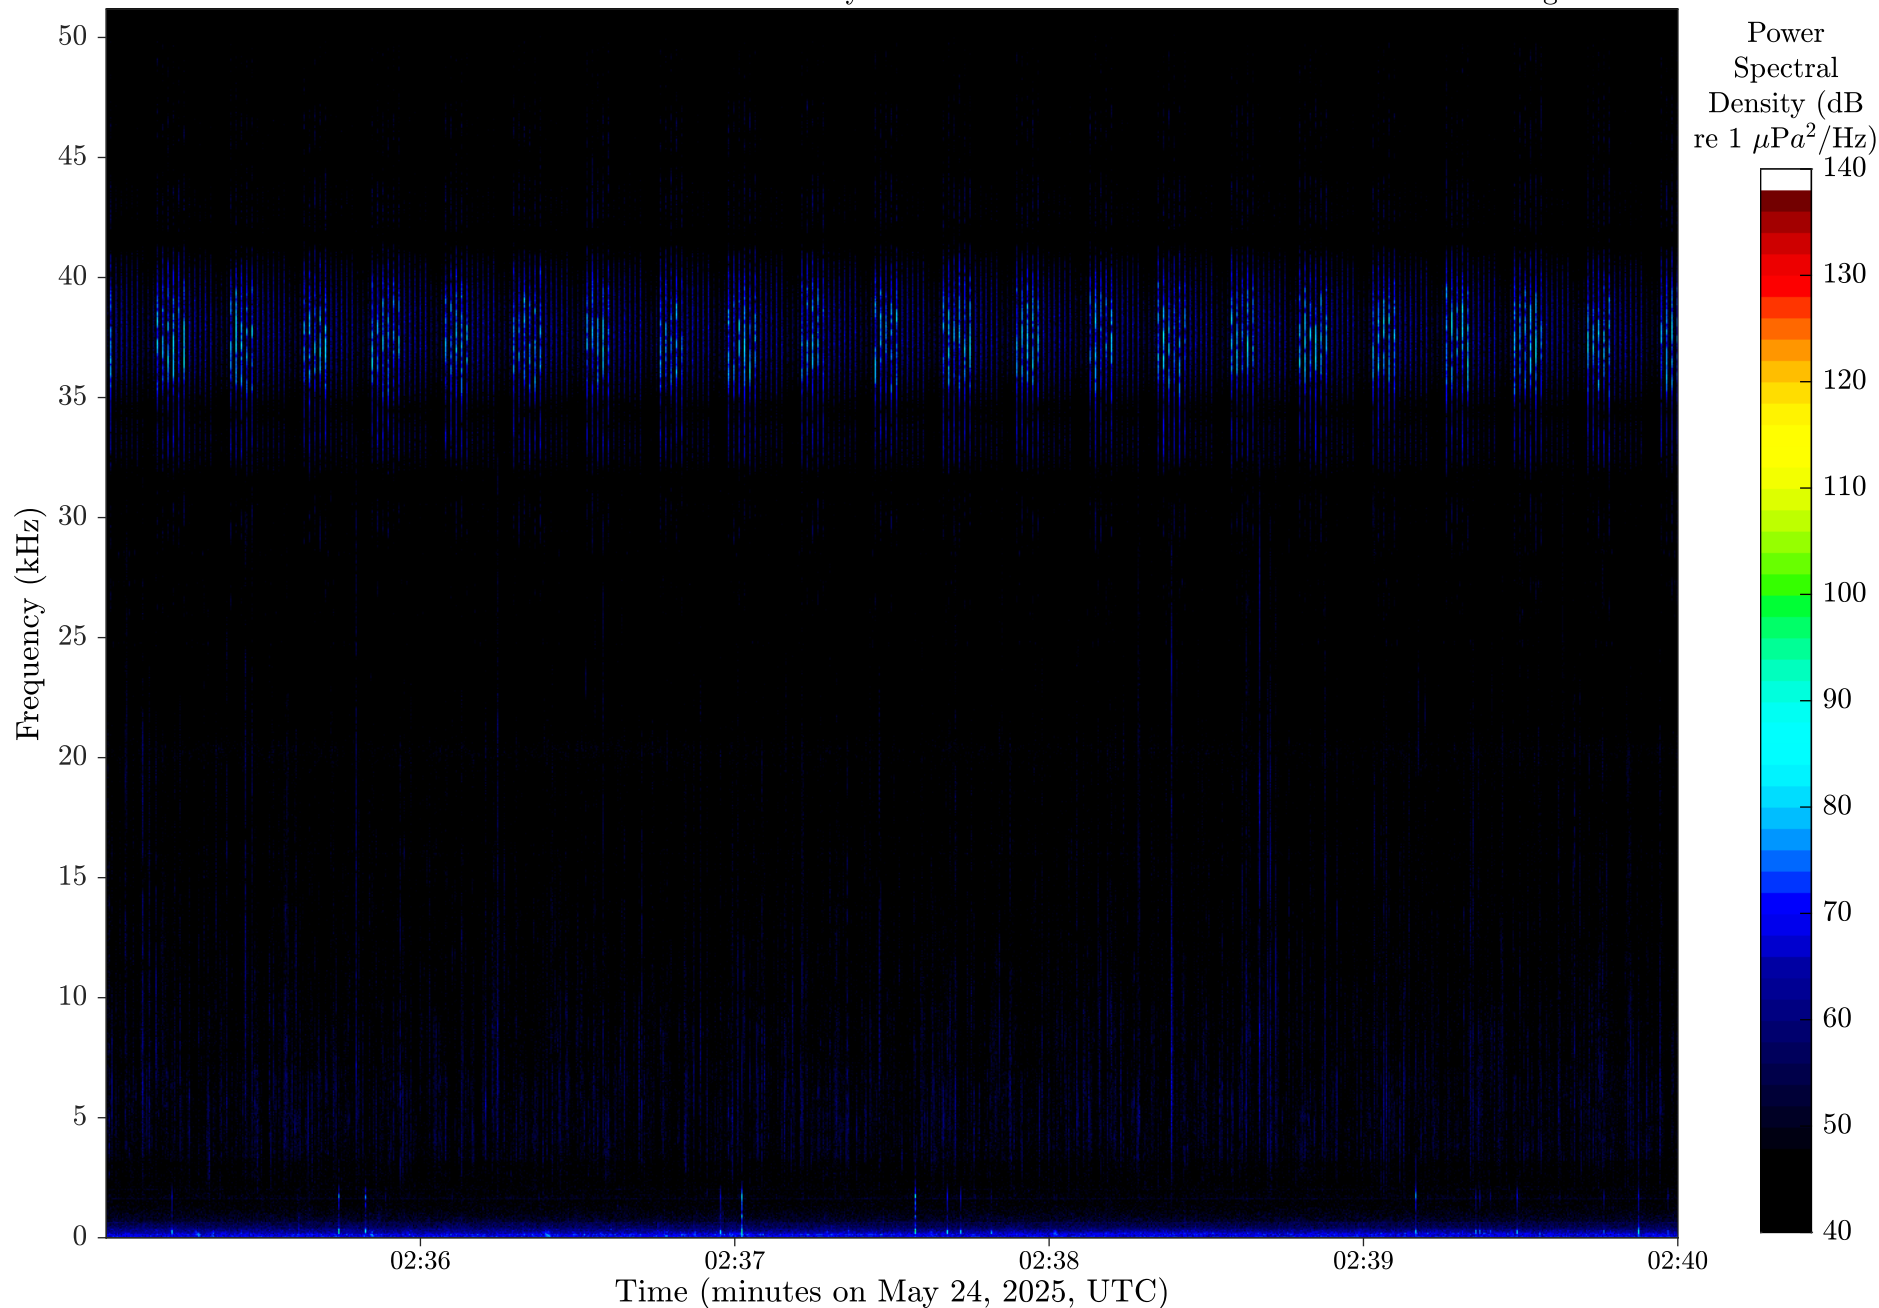

Comments: 36.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:19:10 UTC

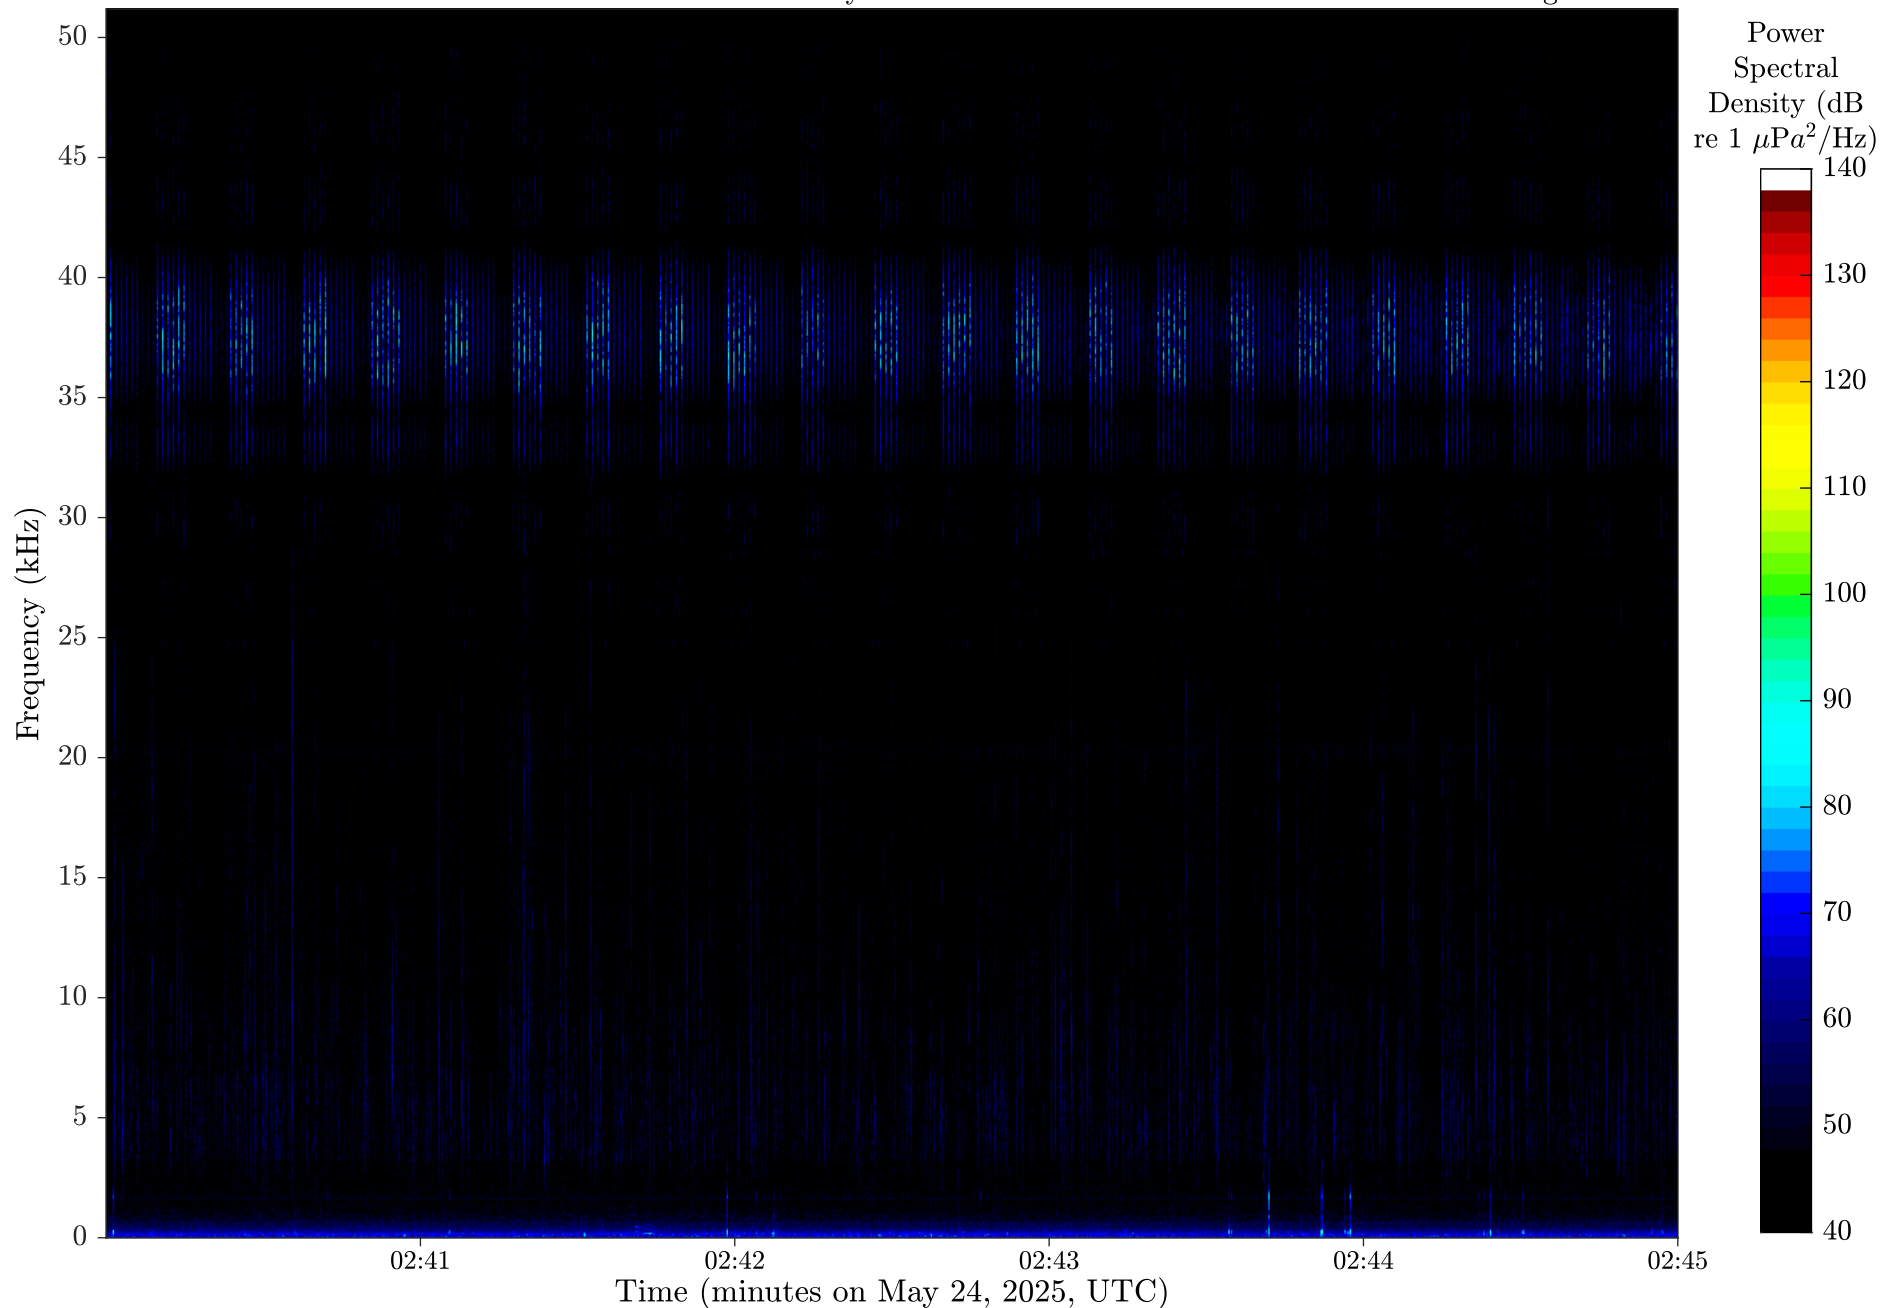

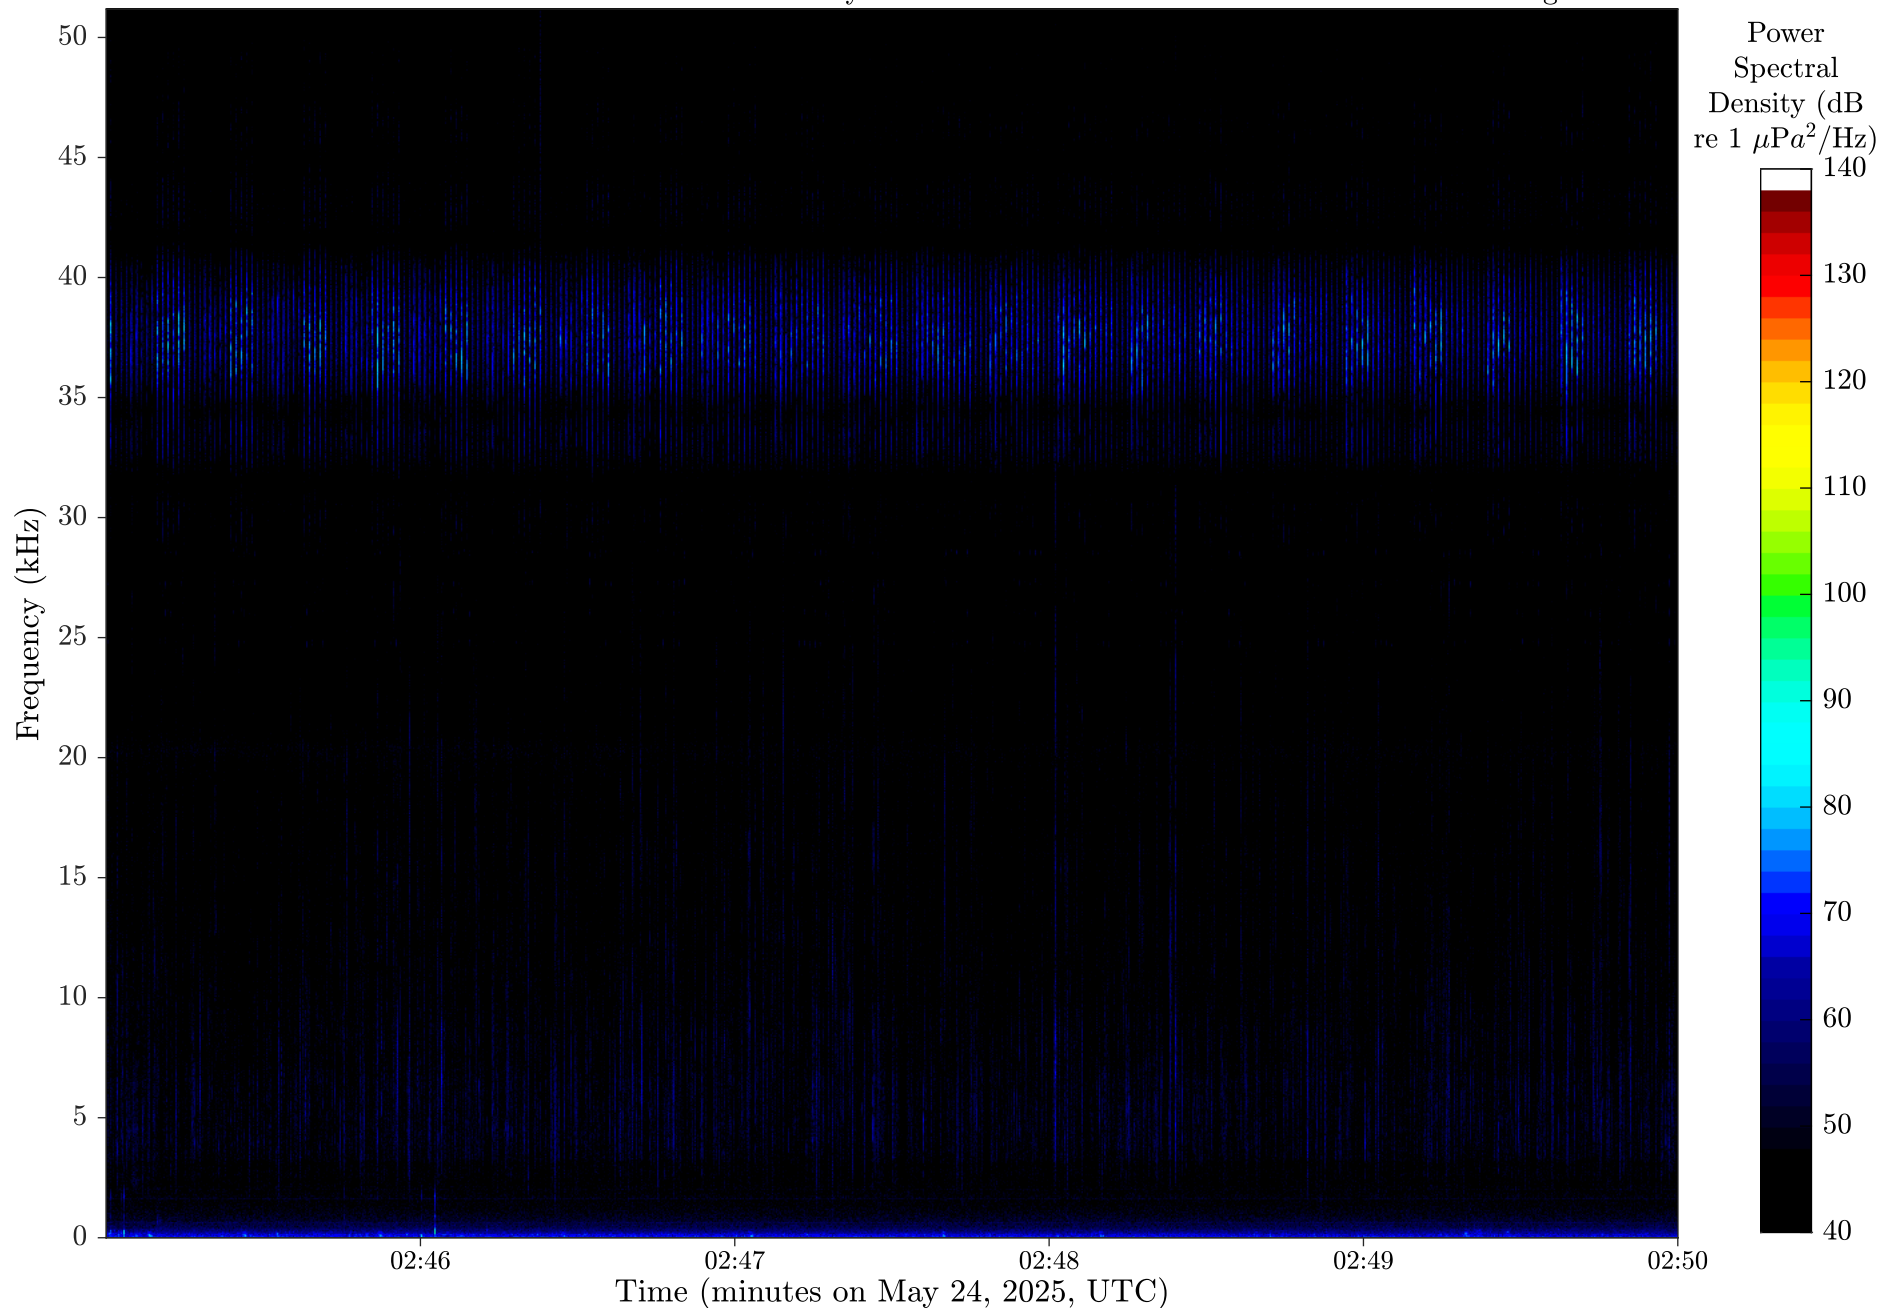


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:19:26 UTC

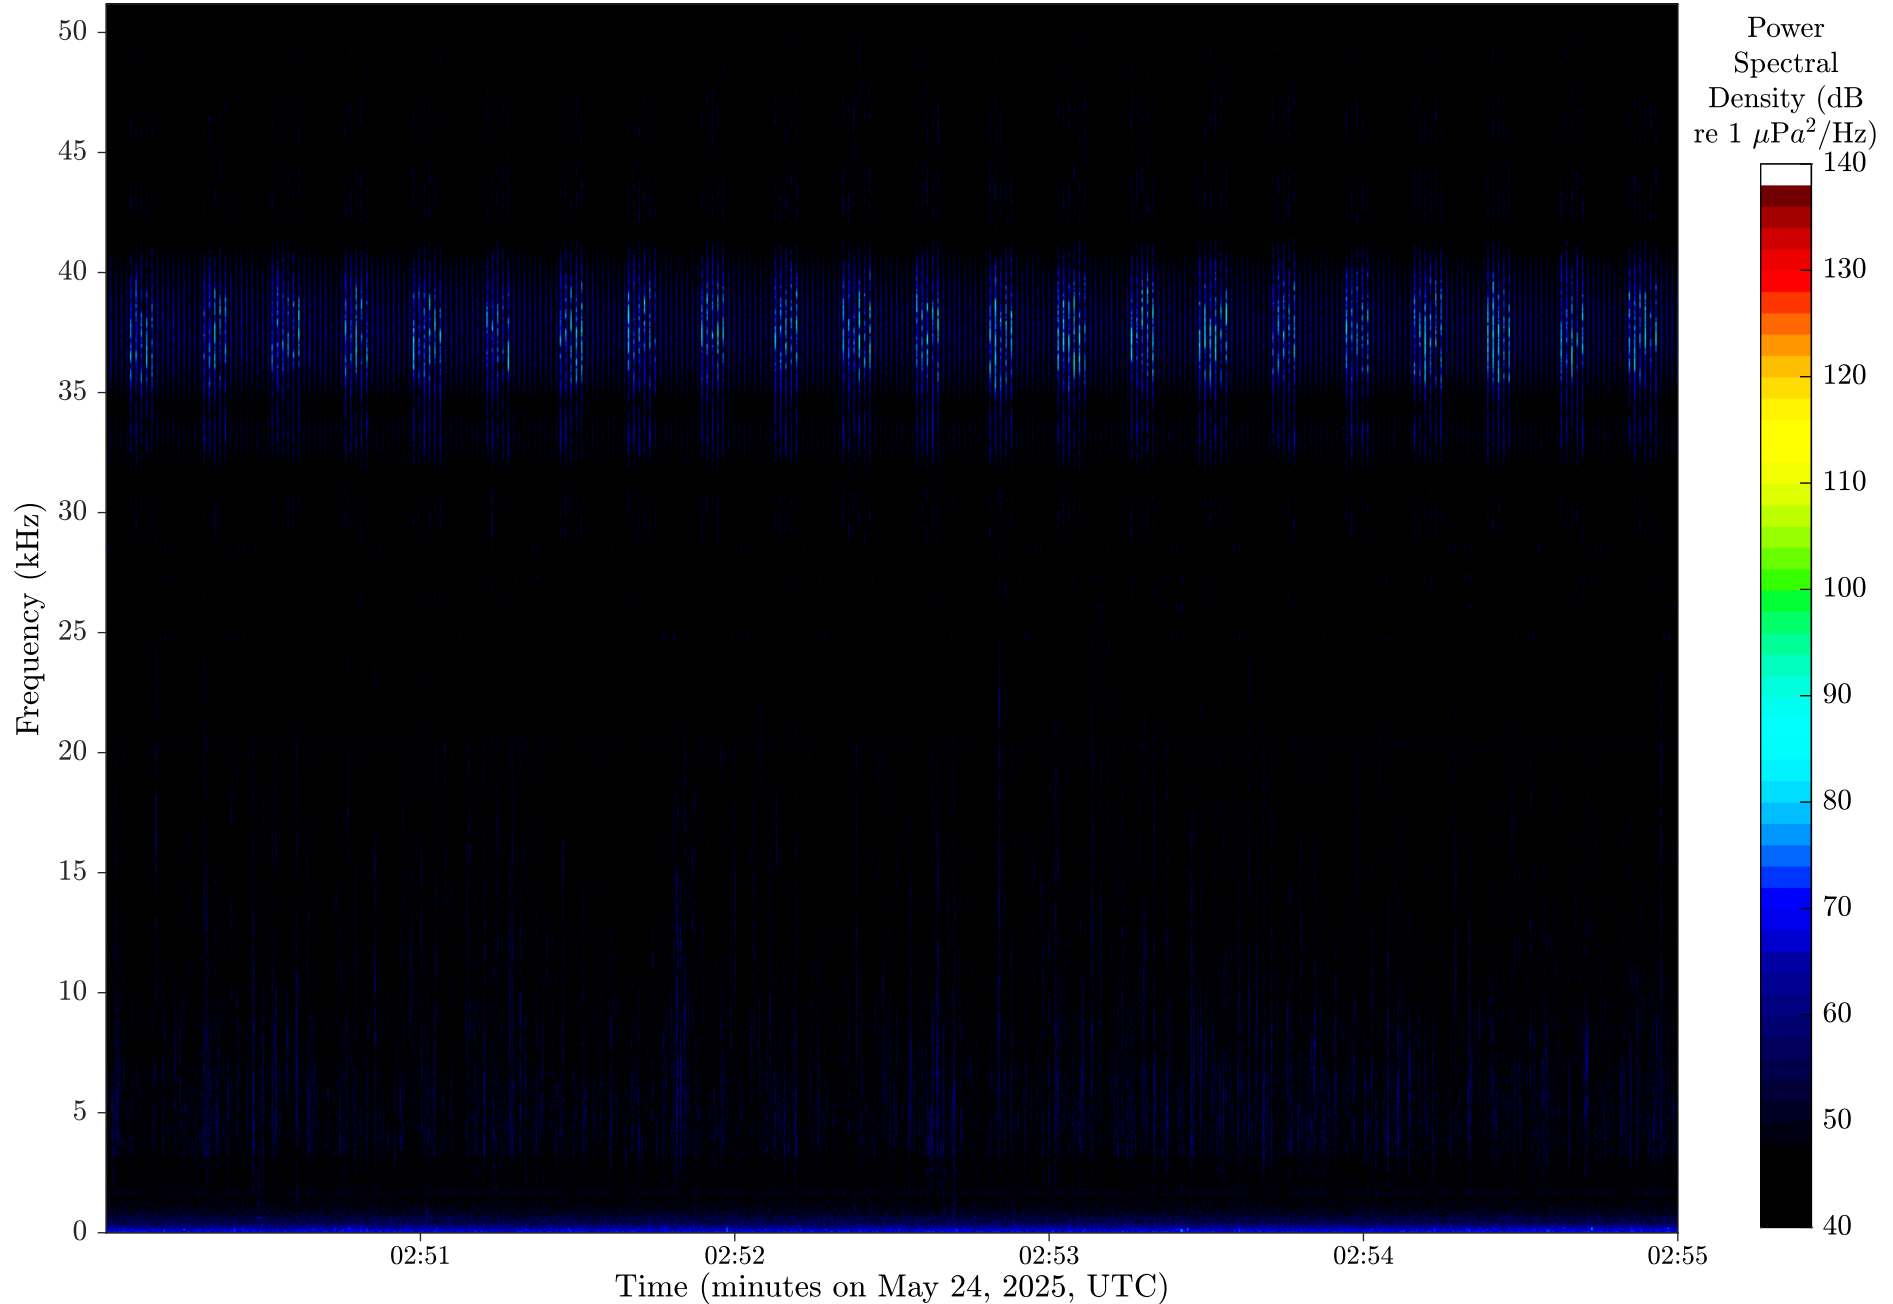


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:19:35 UTC

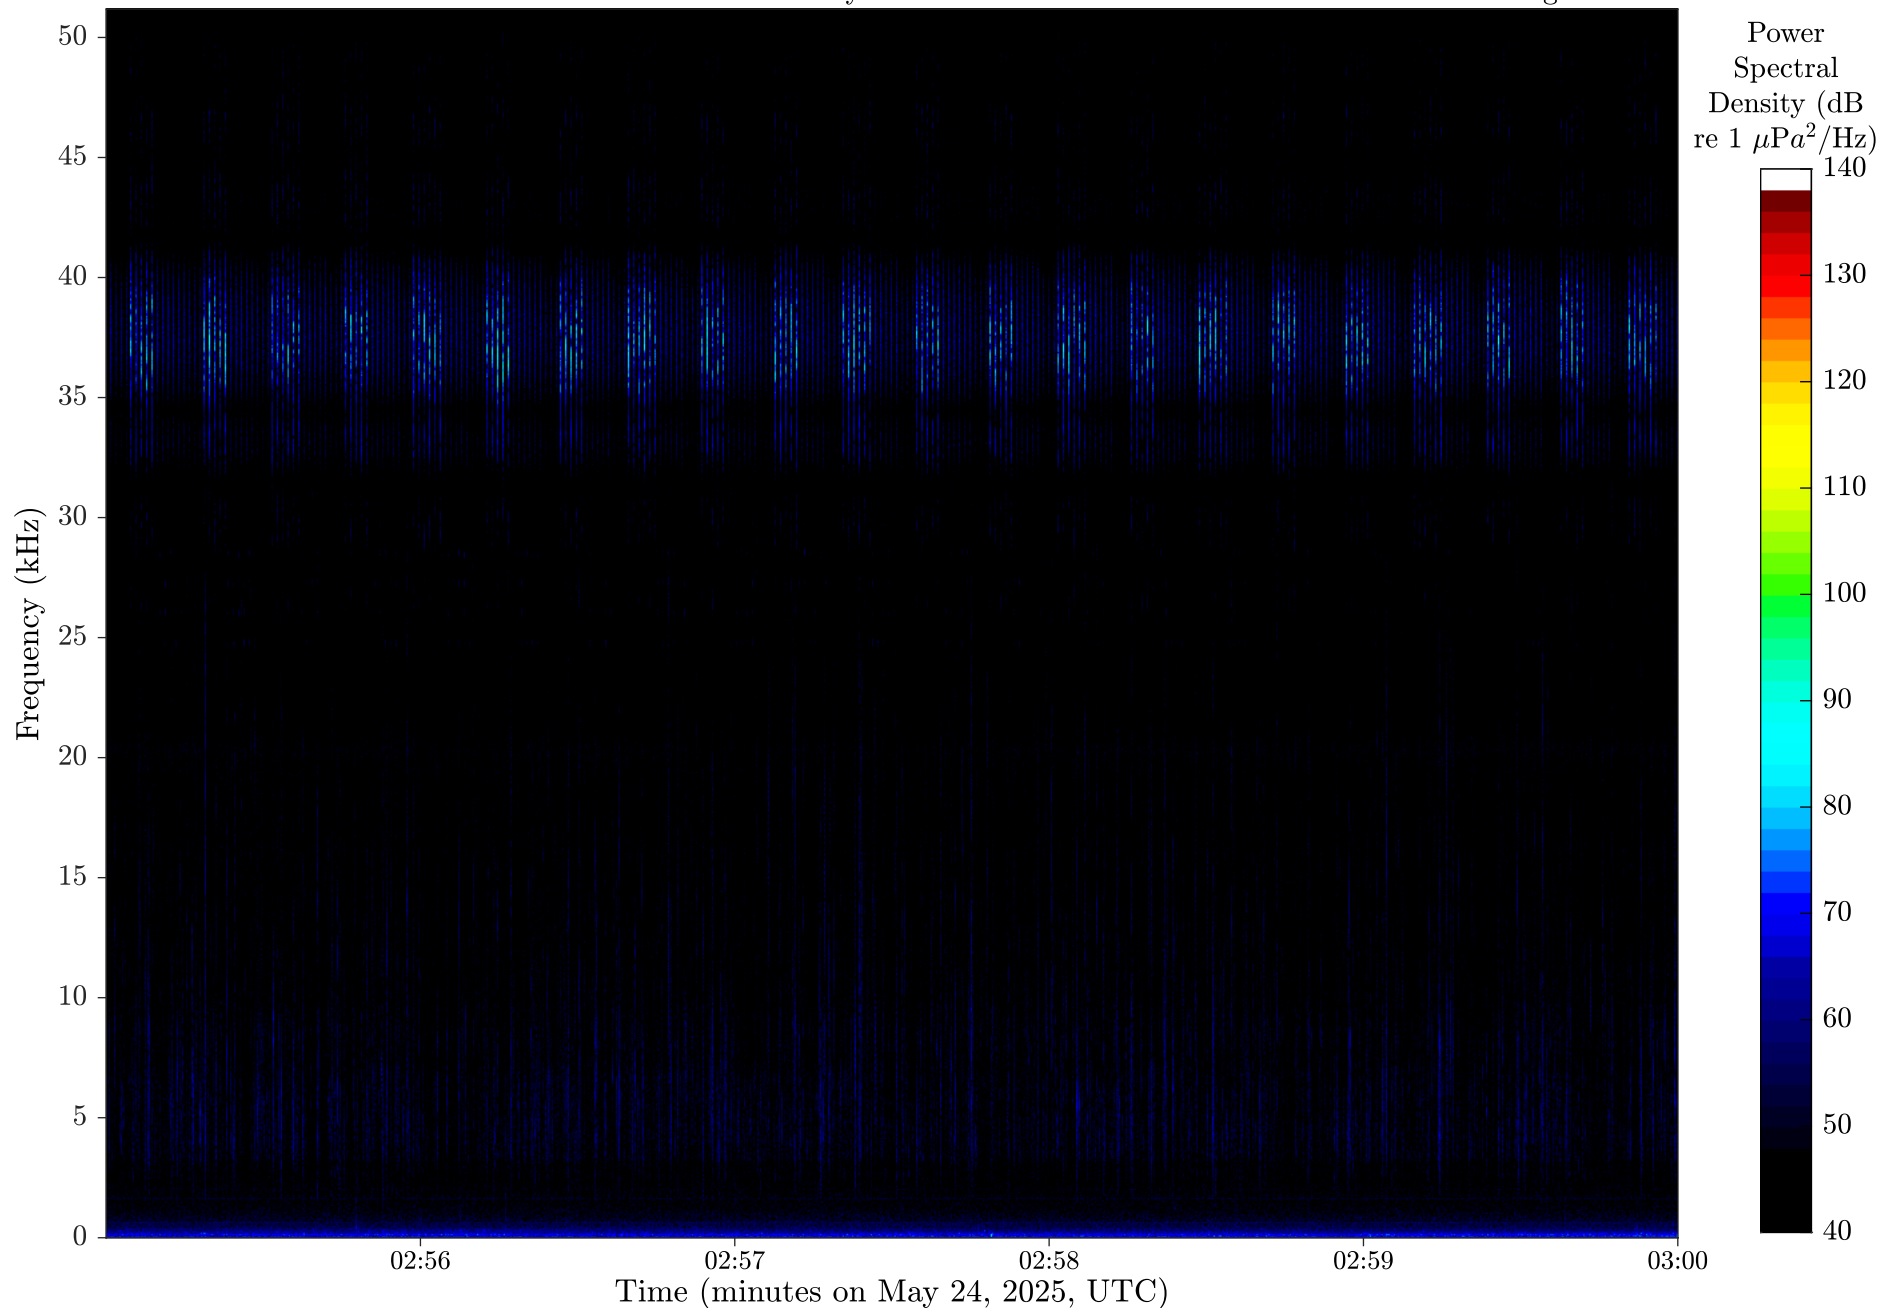


Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:19:43 UTC

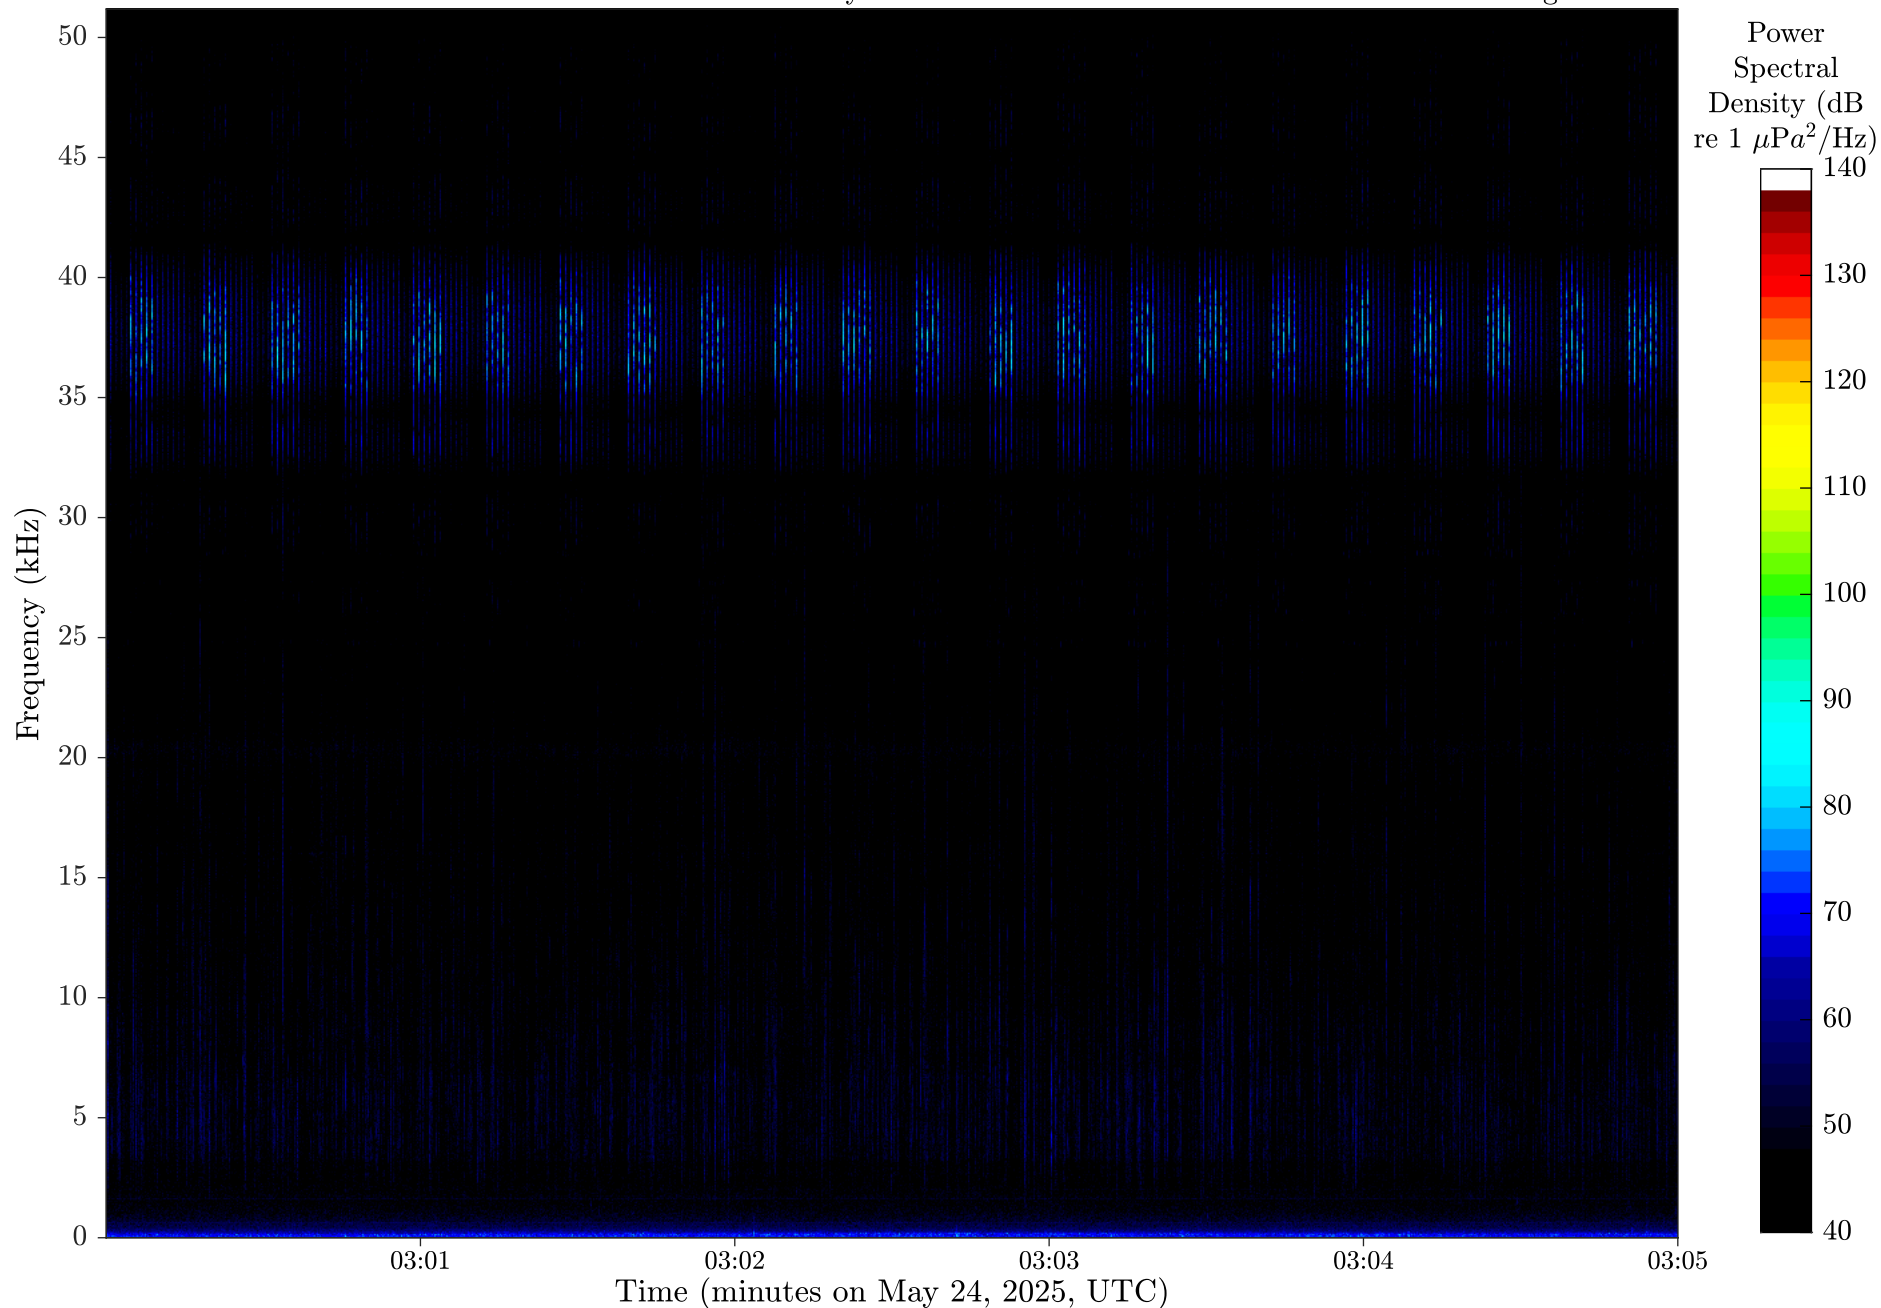


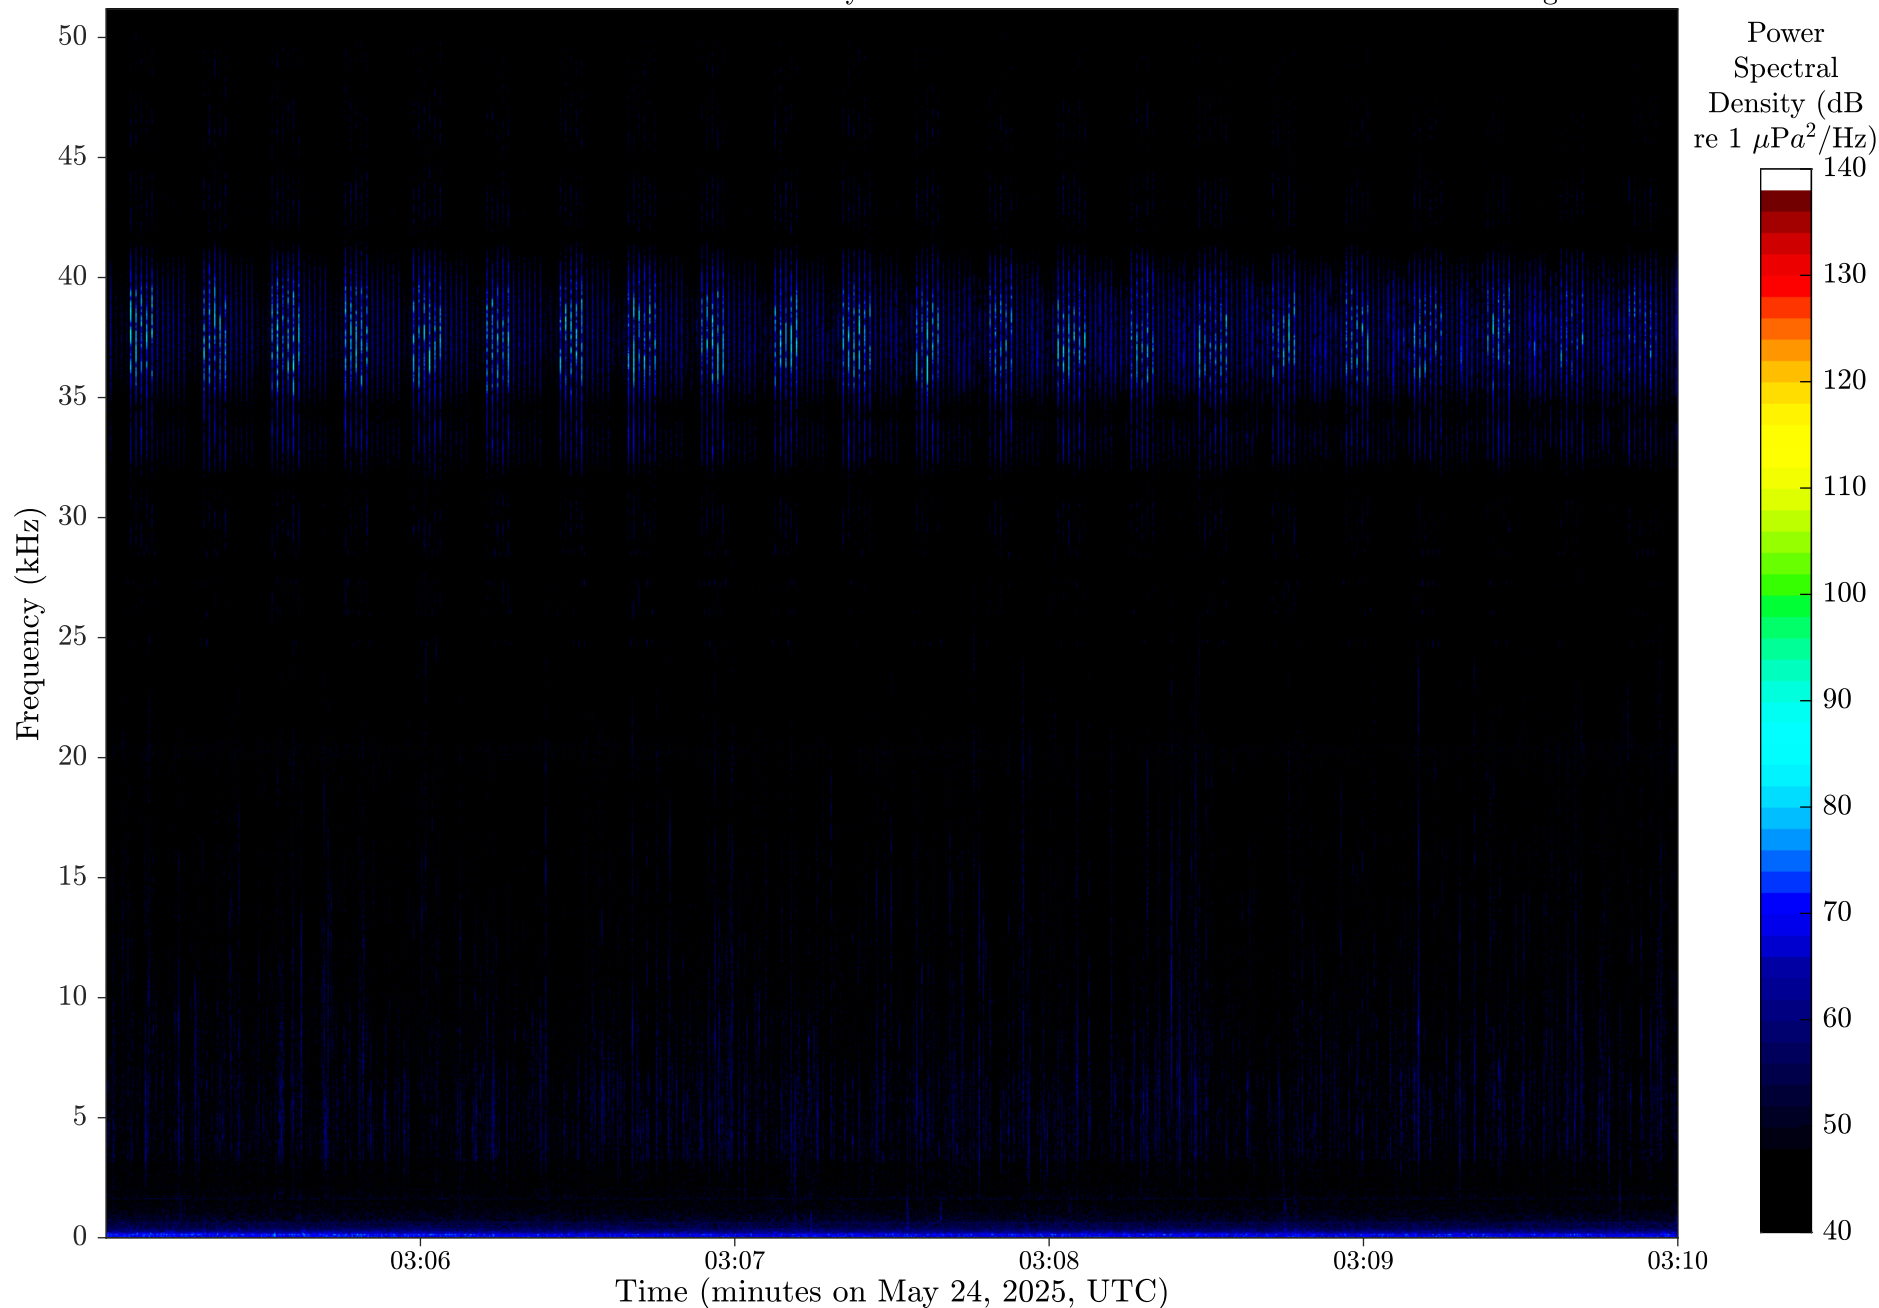

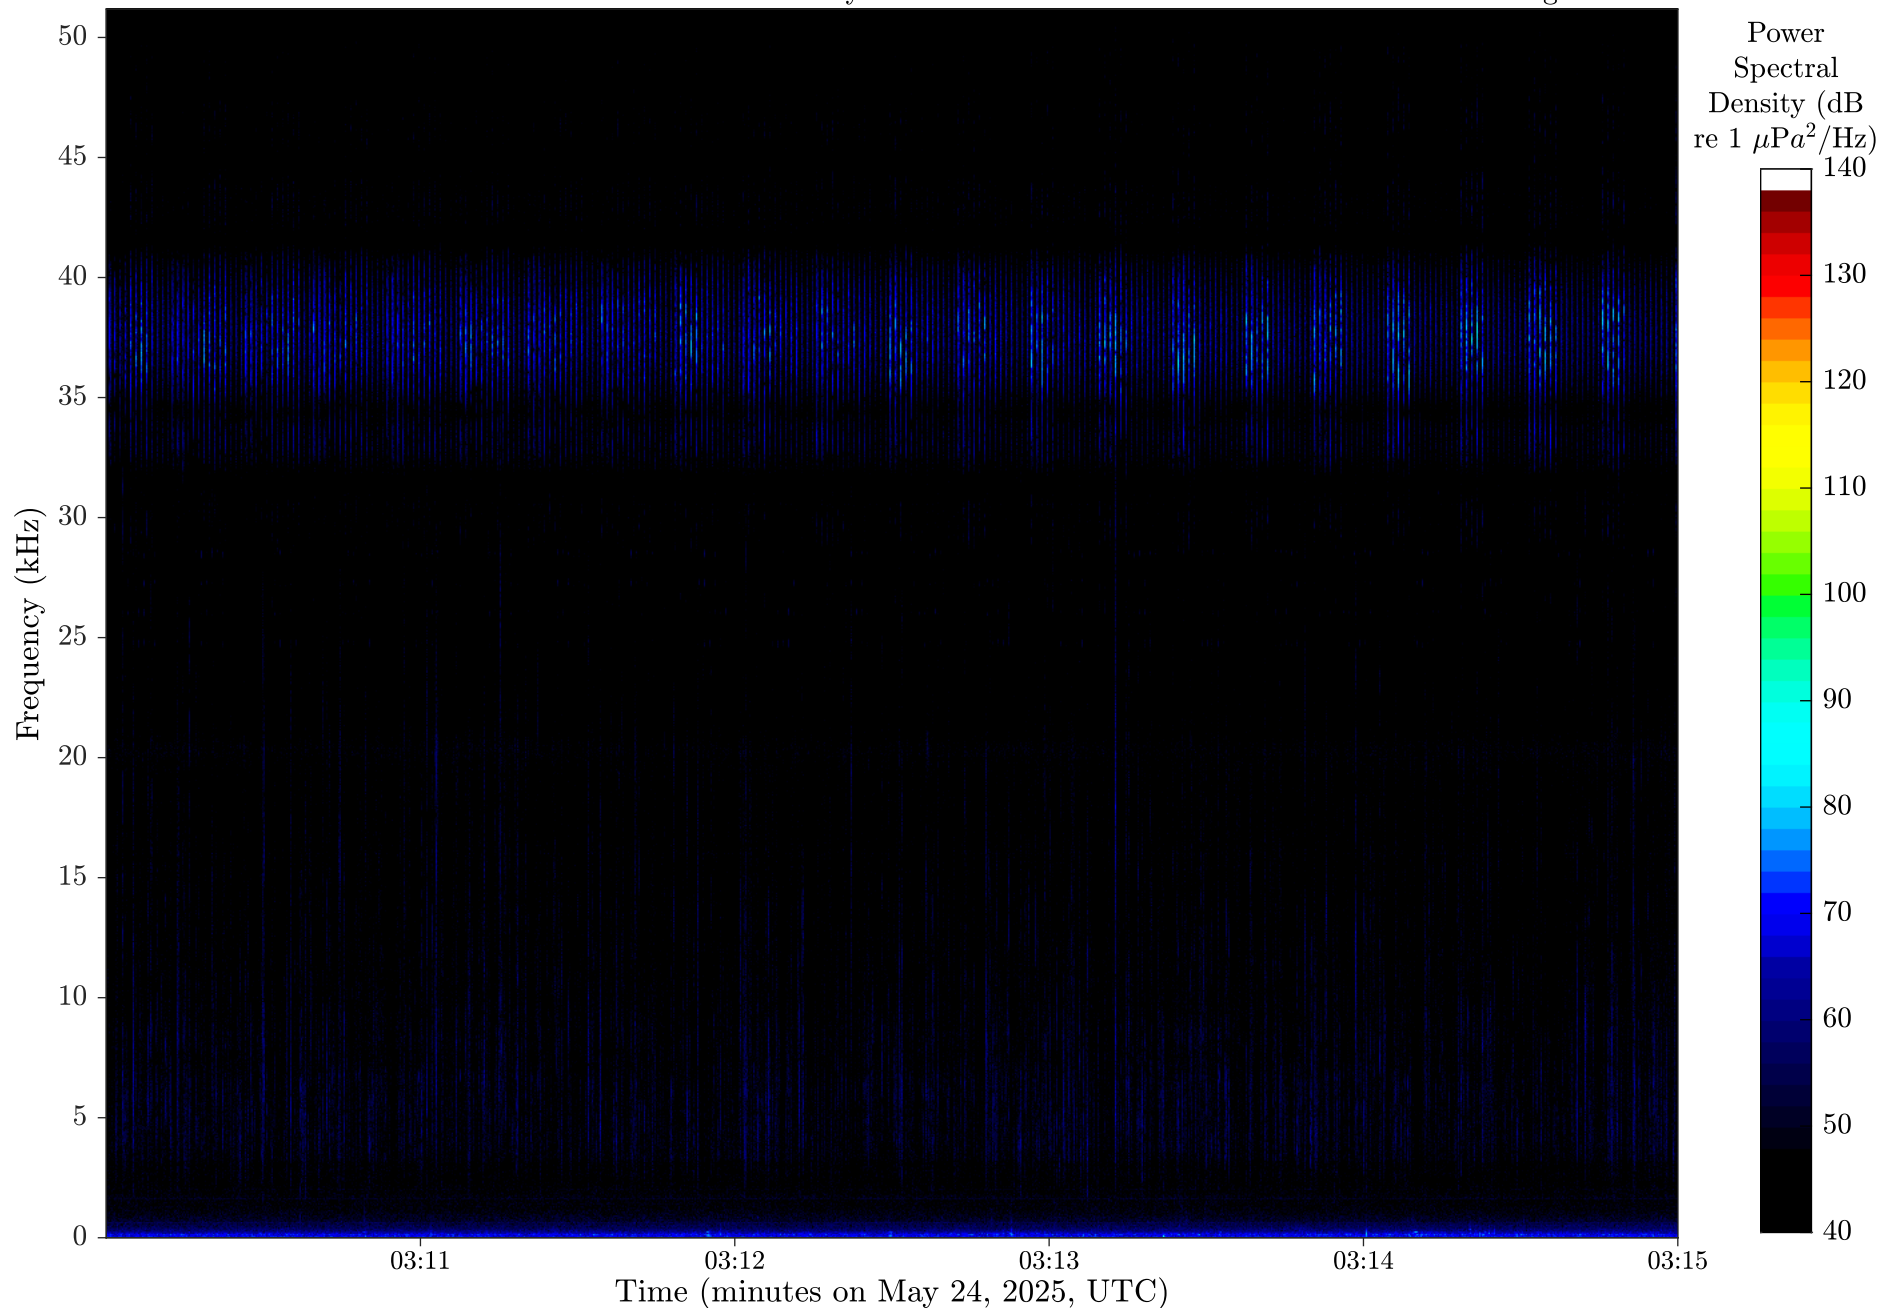


Comments: 33.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:09 UTC

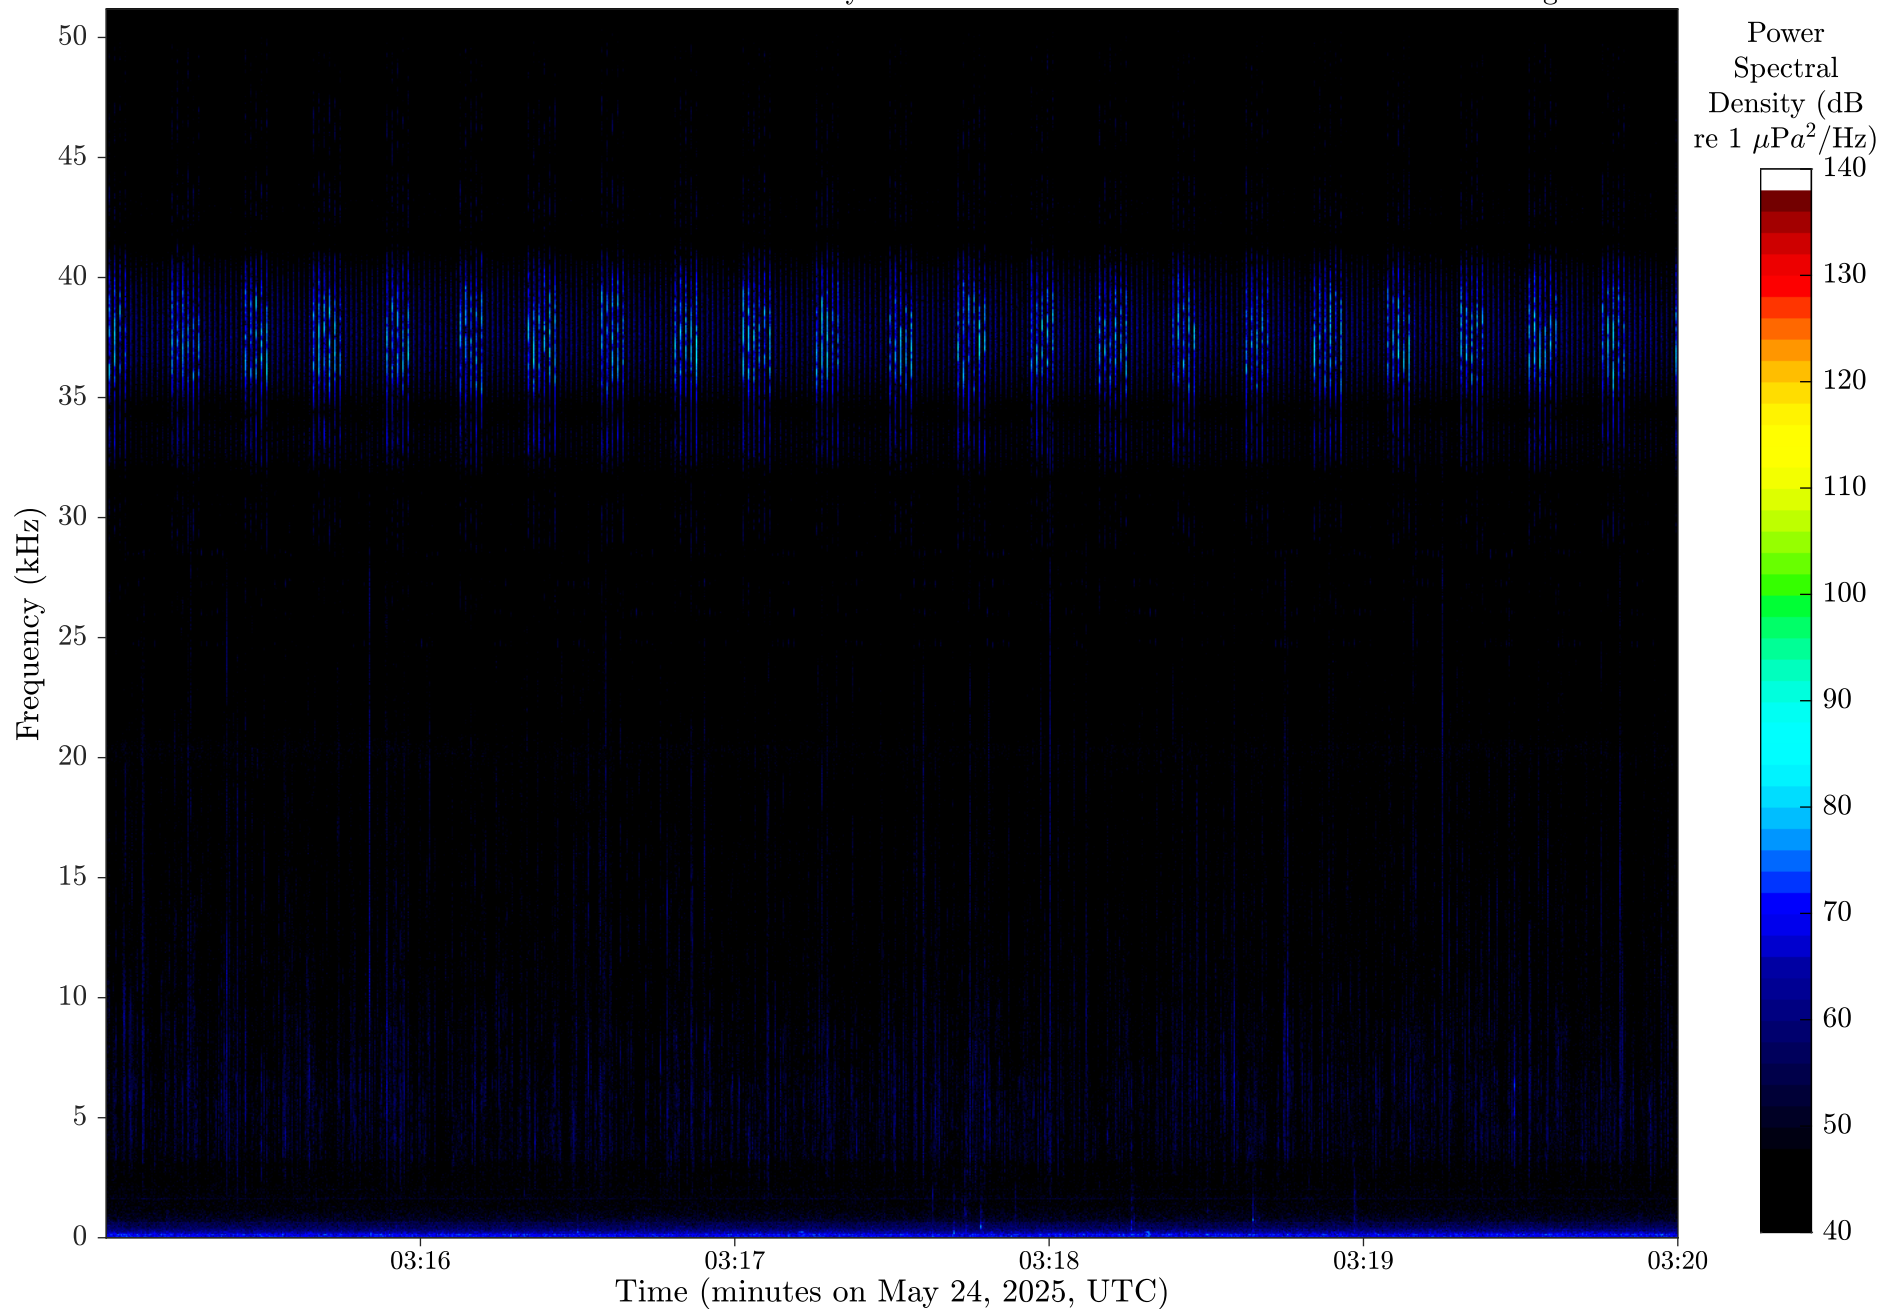


Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:17 UTC

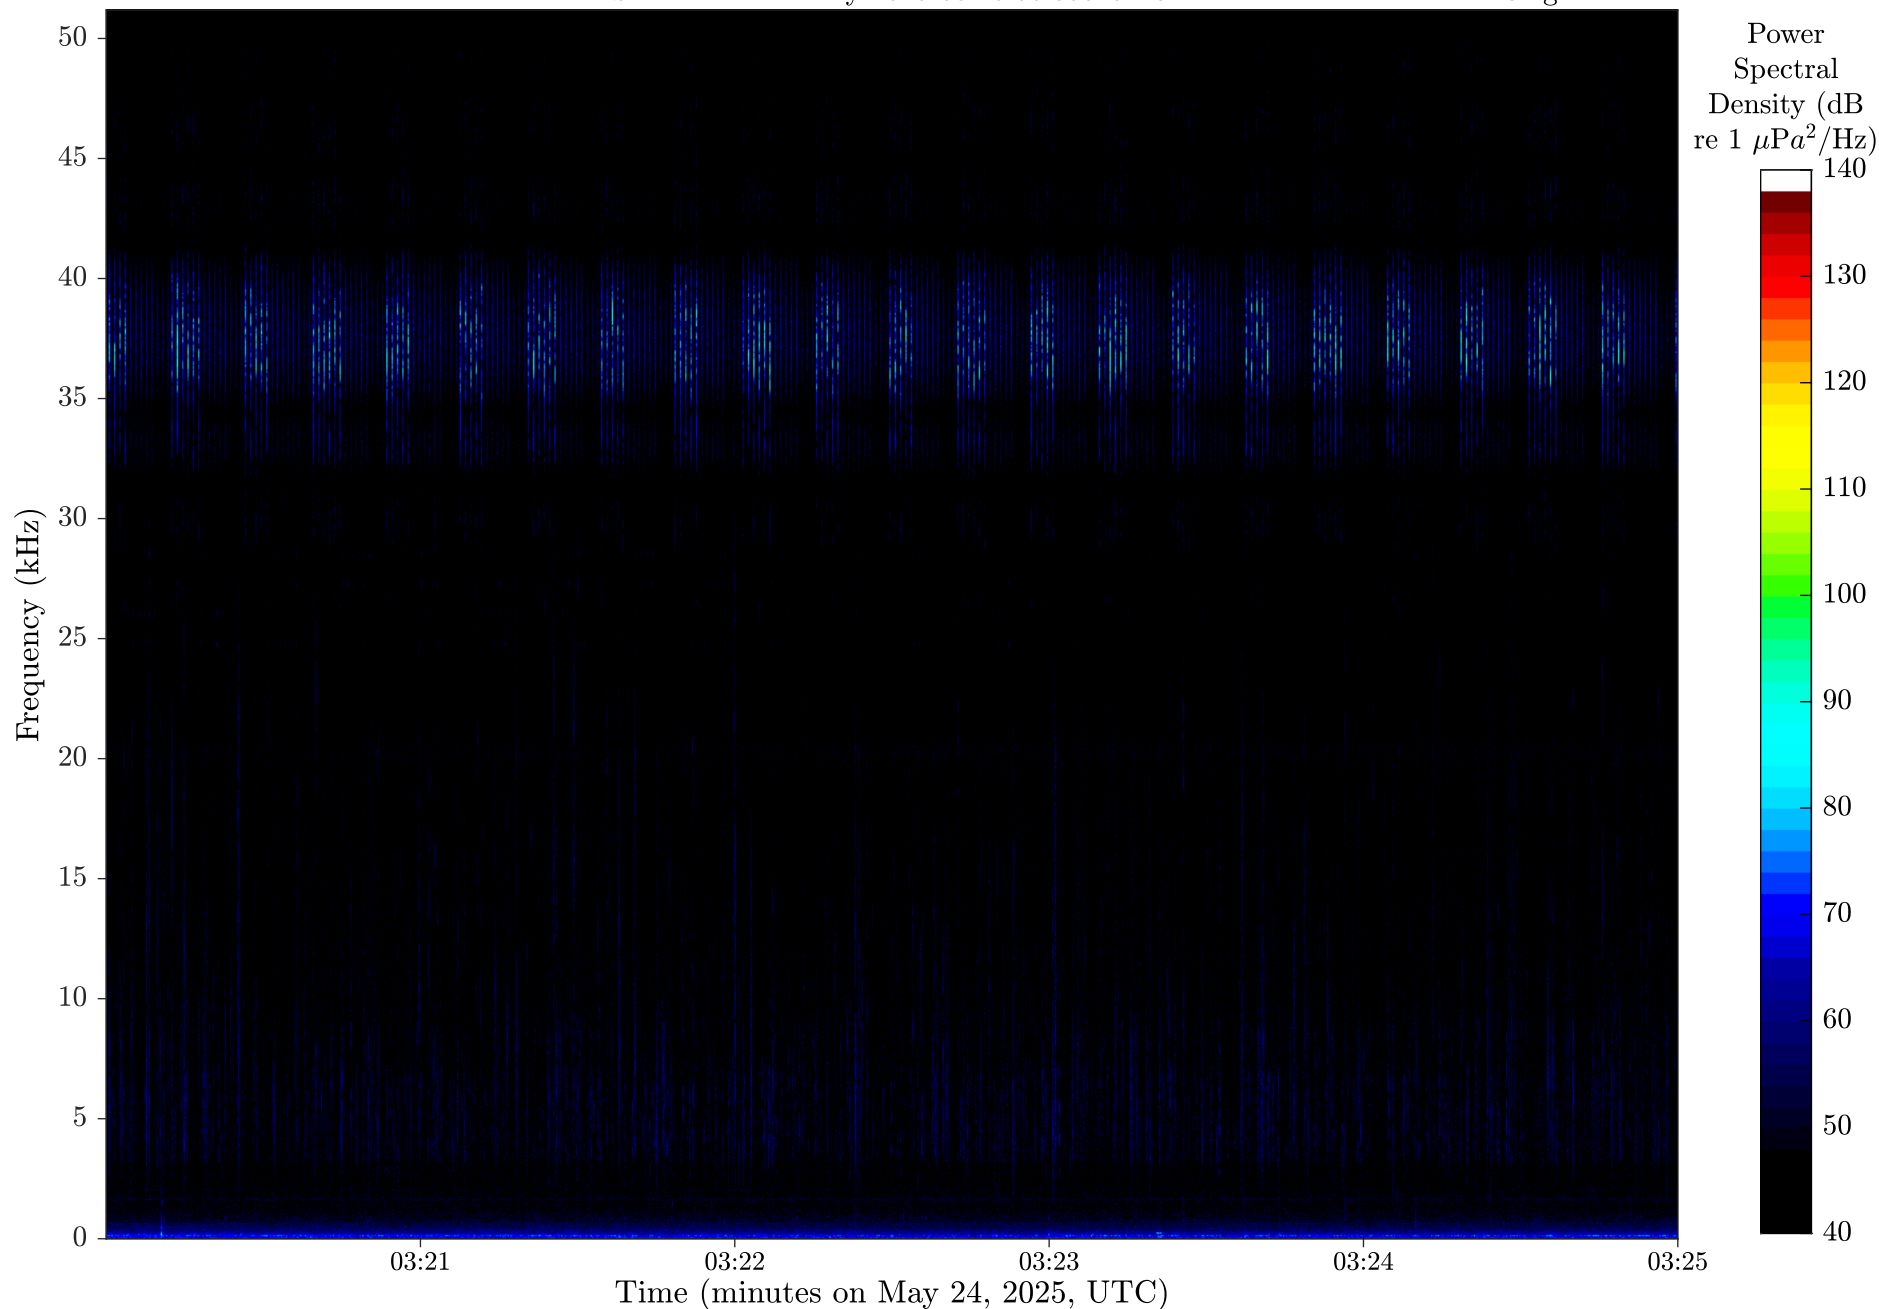


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:25 UTC

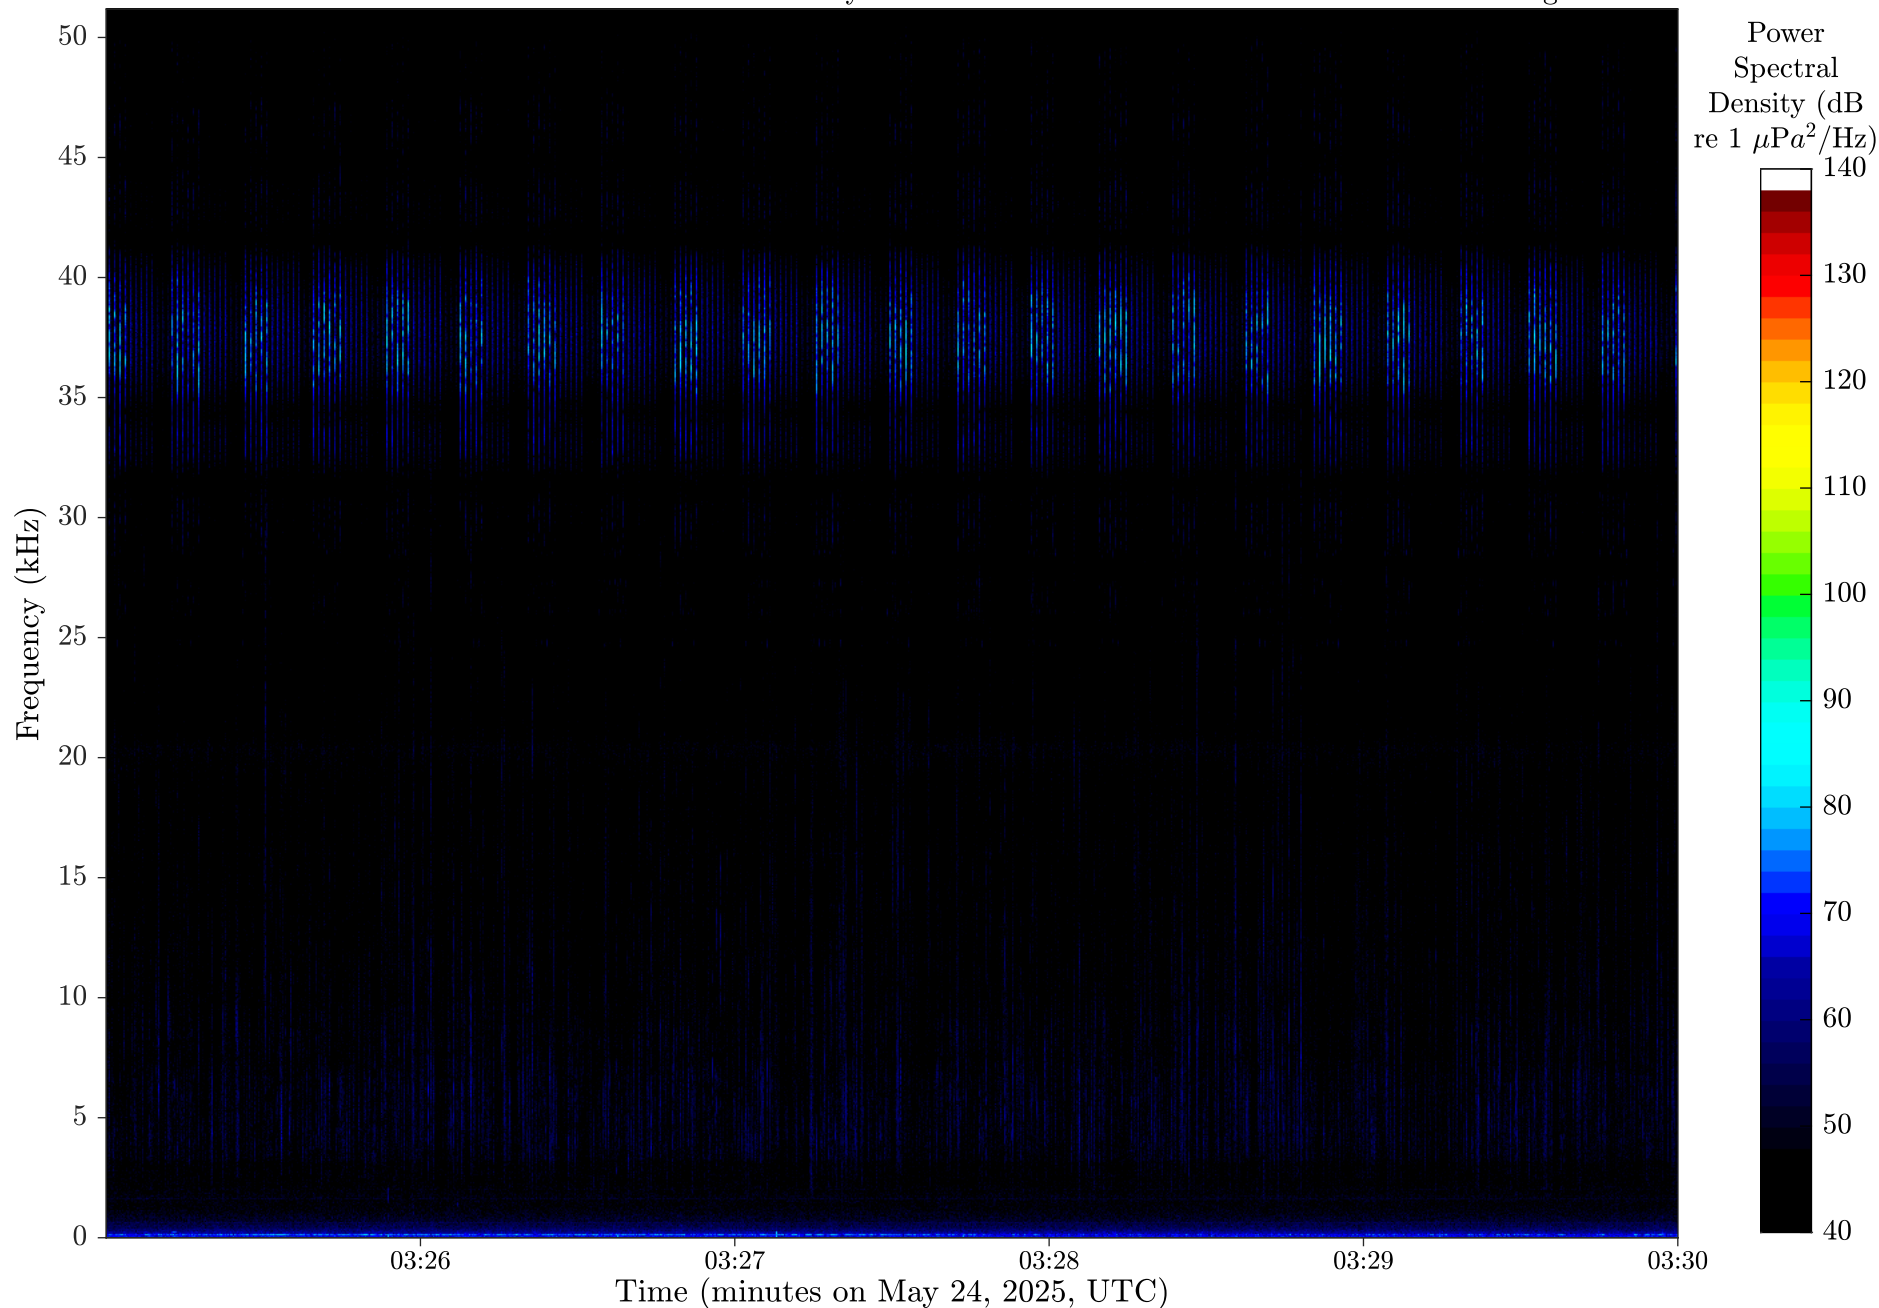


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:33 UTC

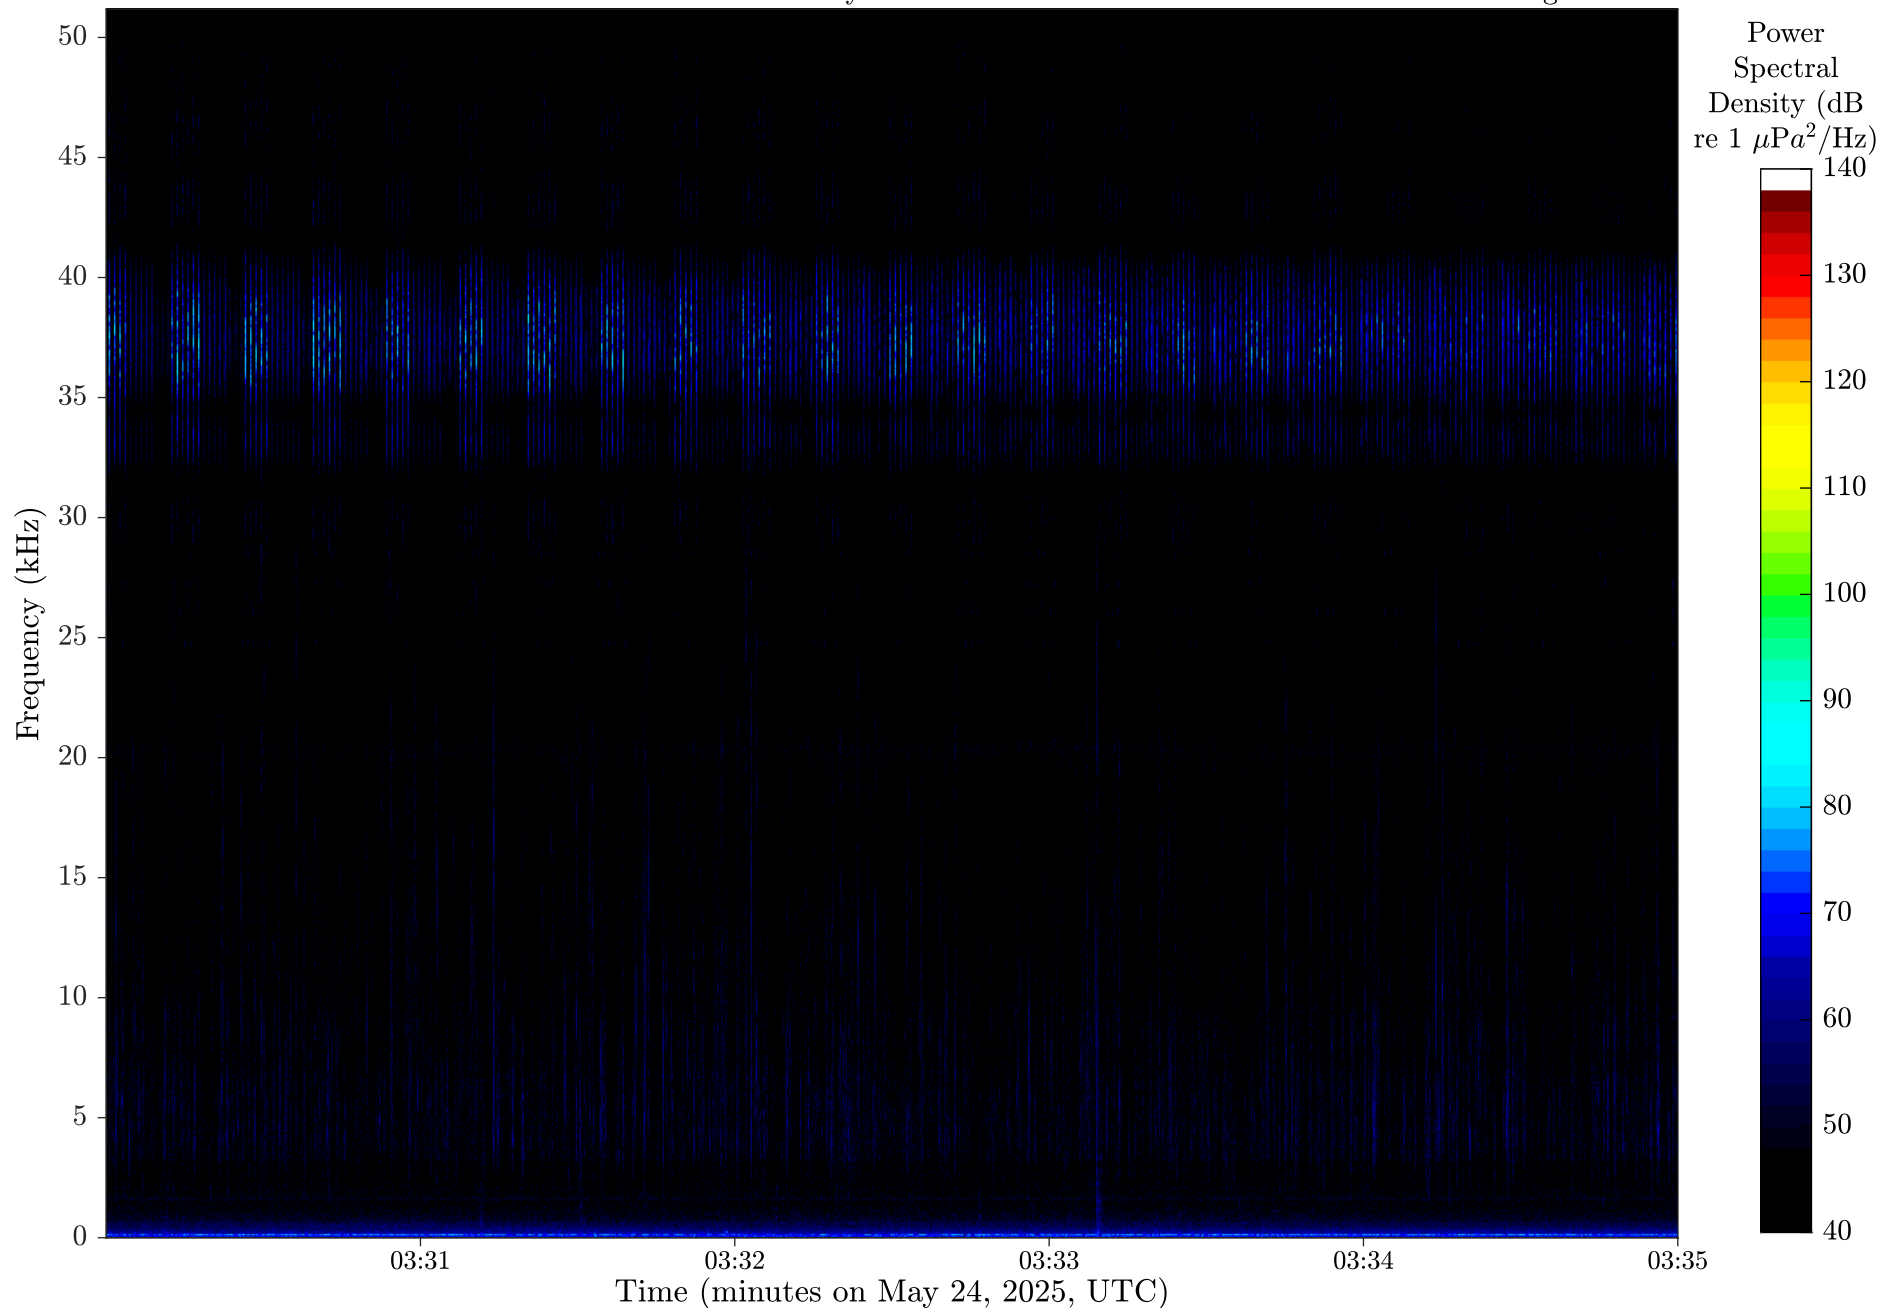


Comments: 34.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:42 UTC

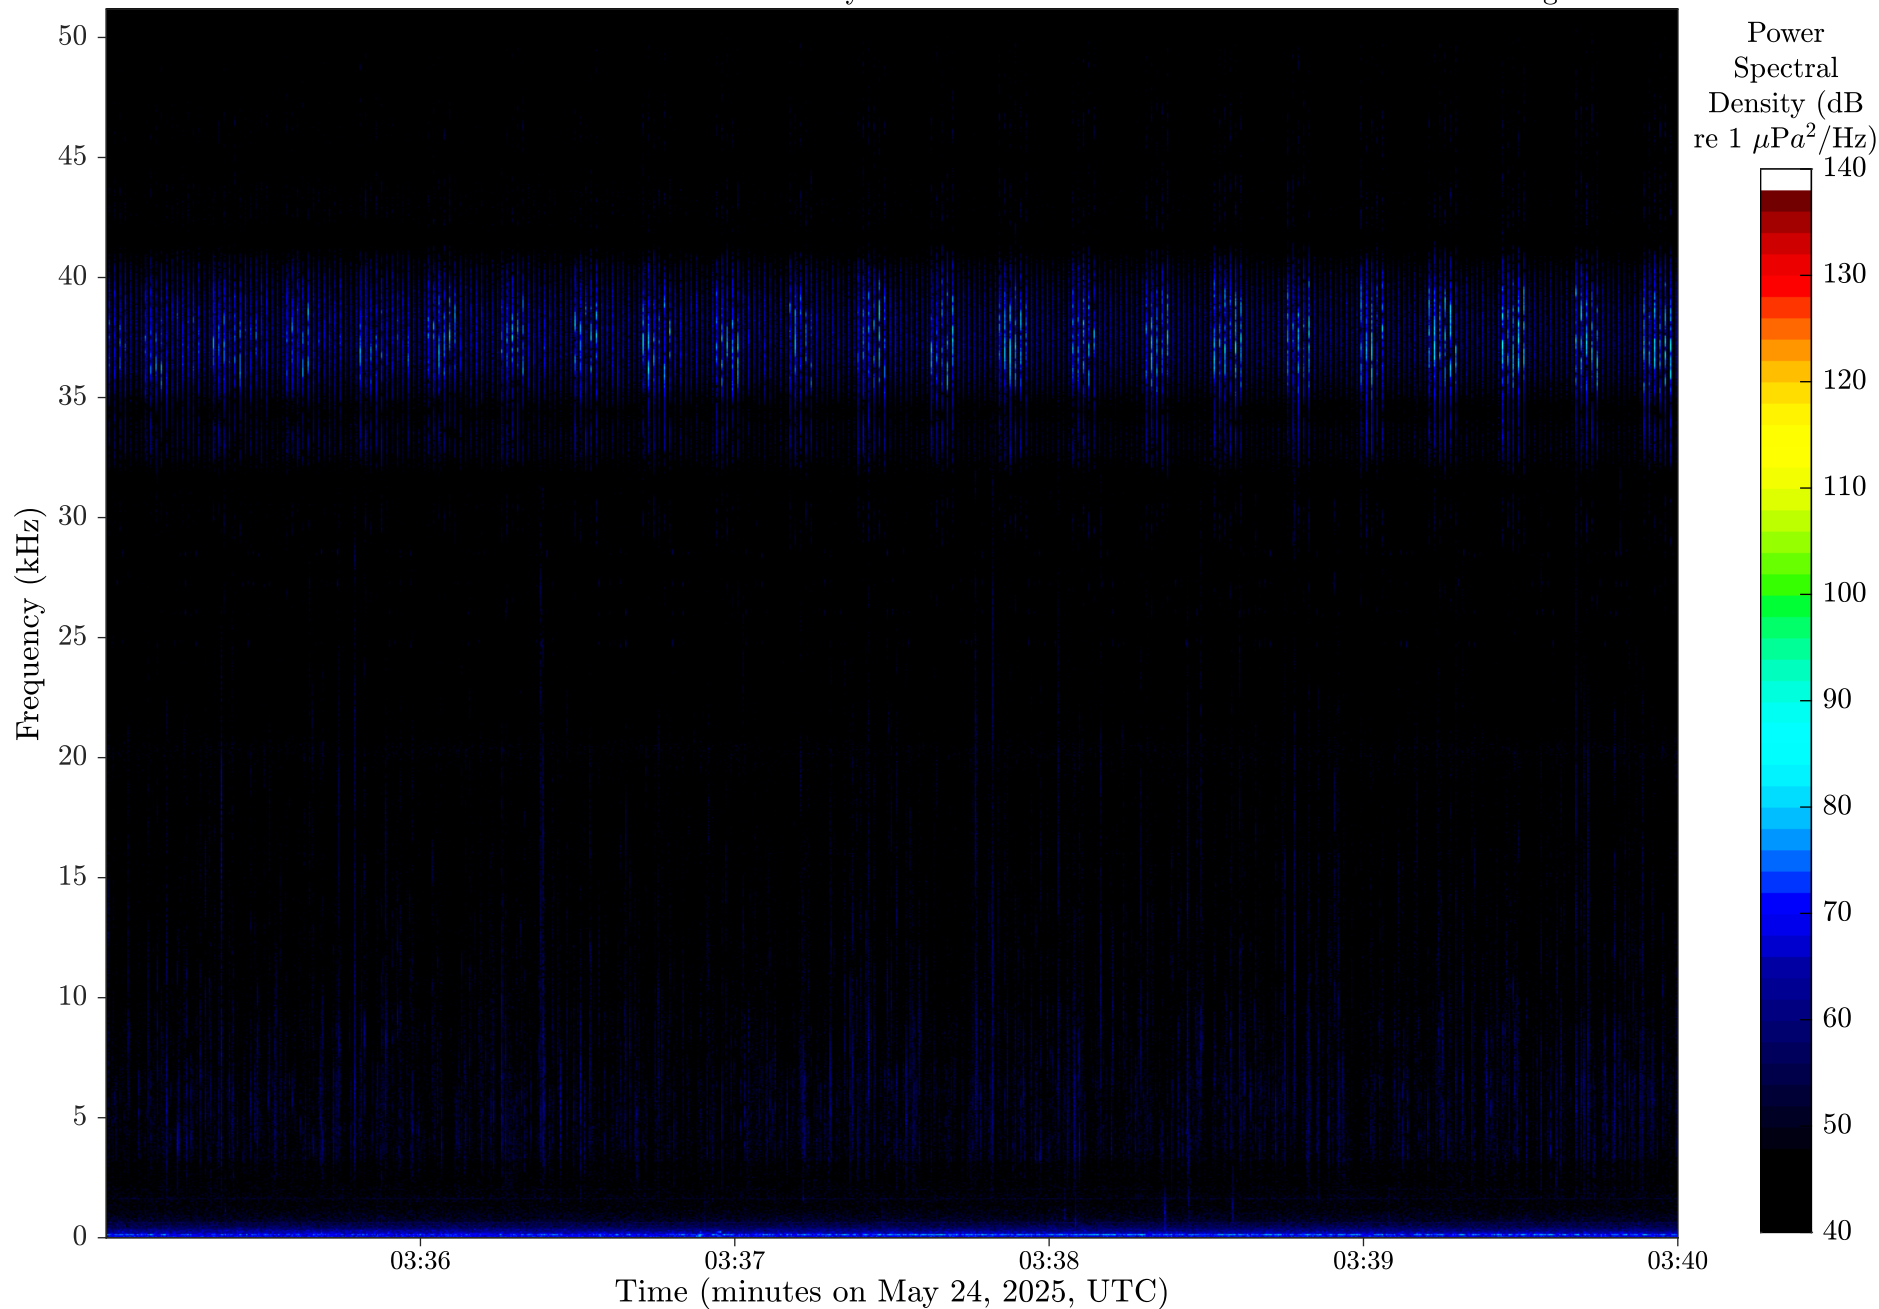


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:50 UTC

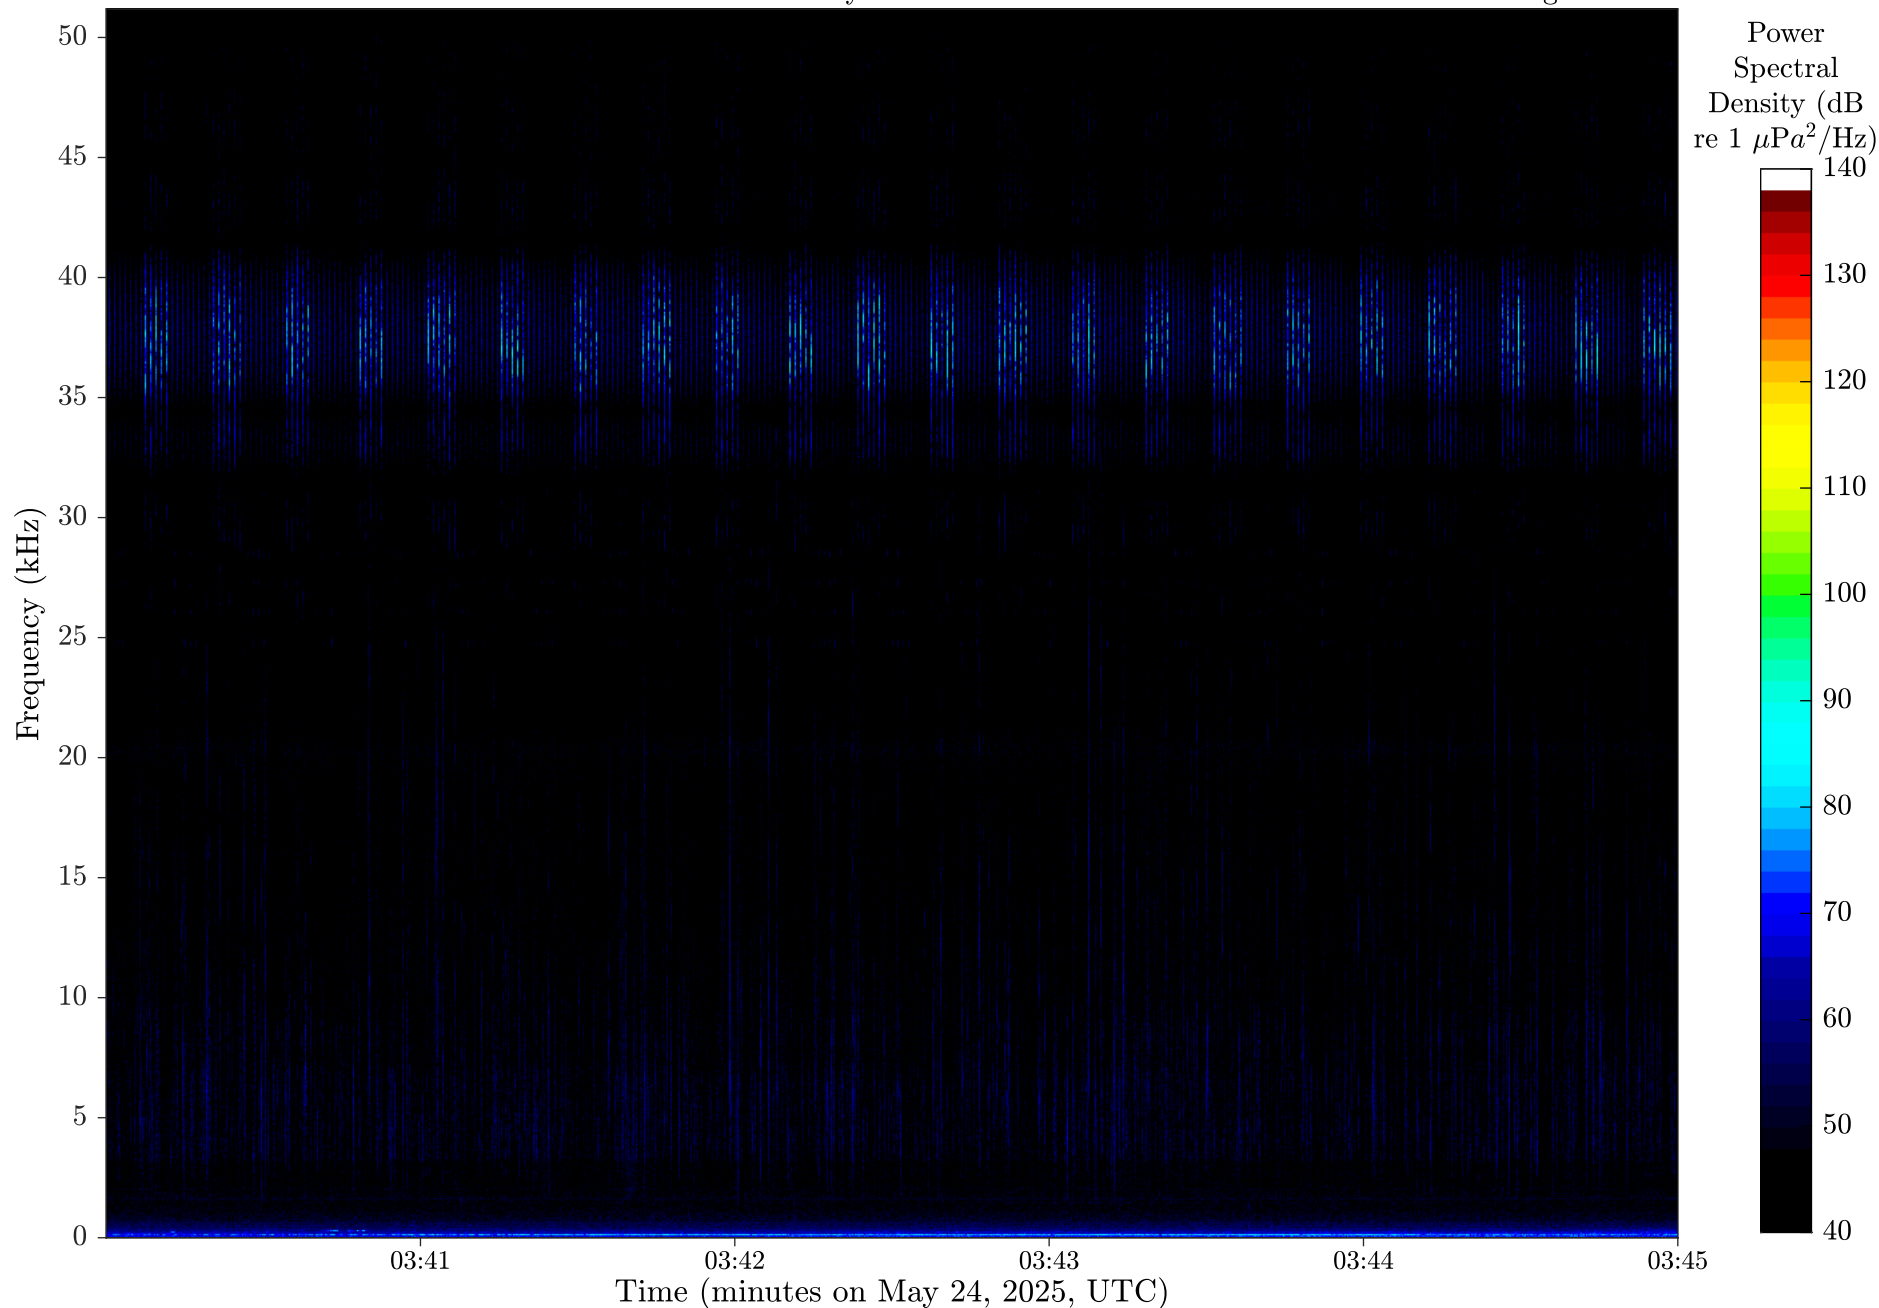


Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:58 UTC

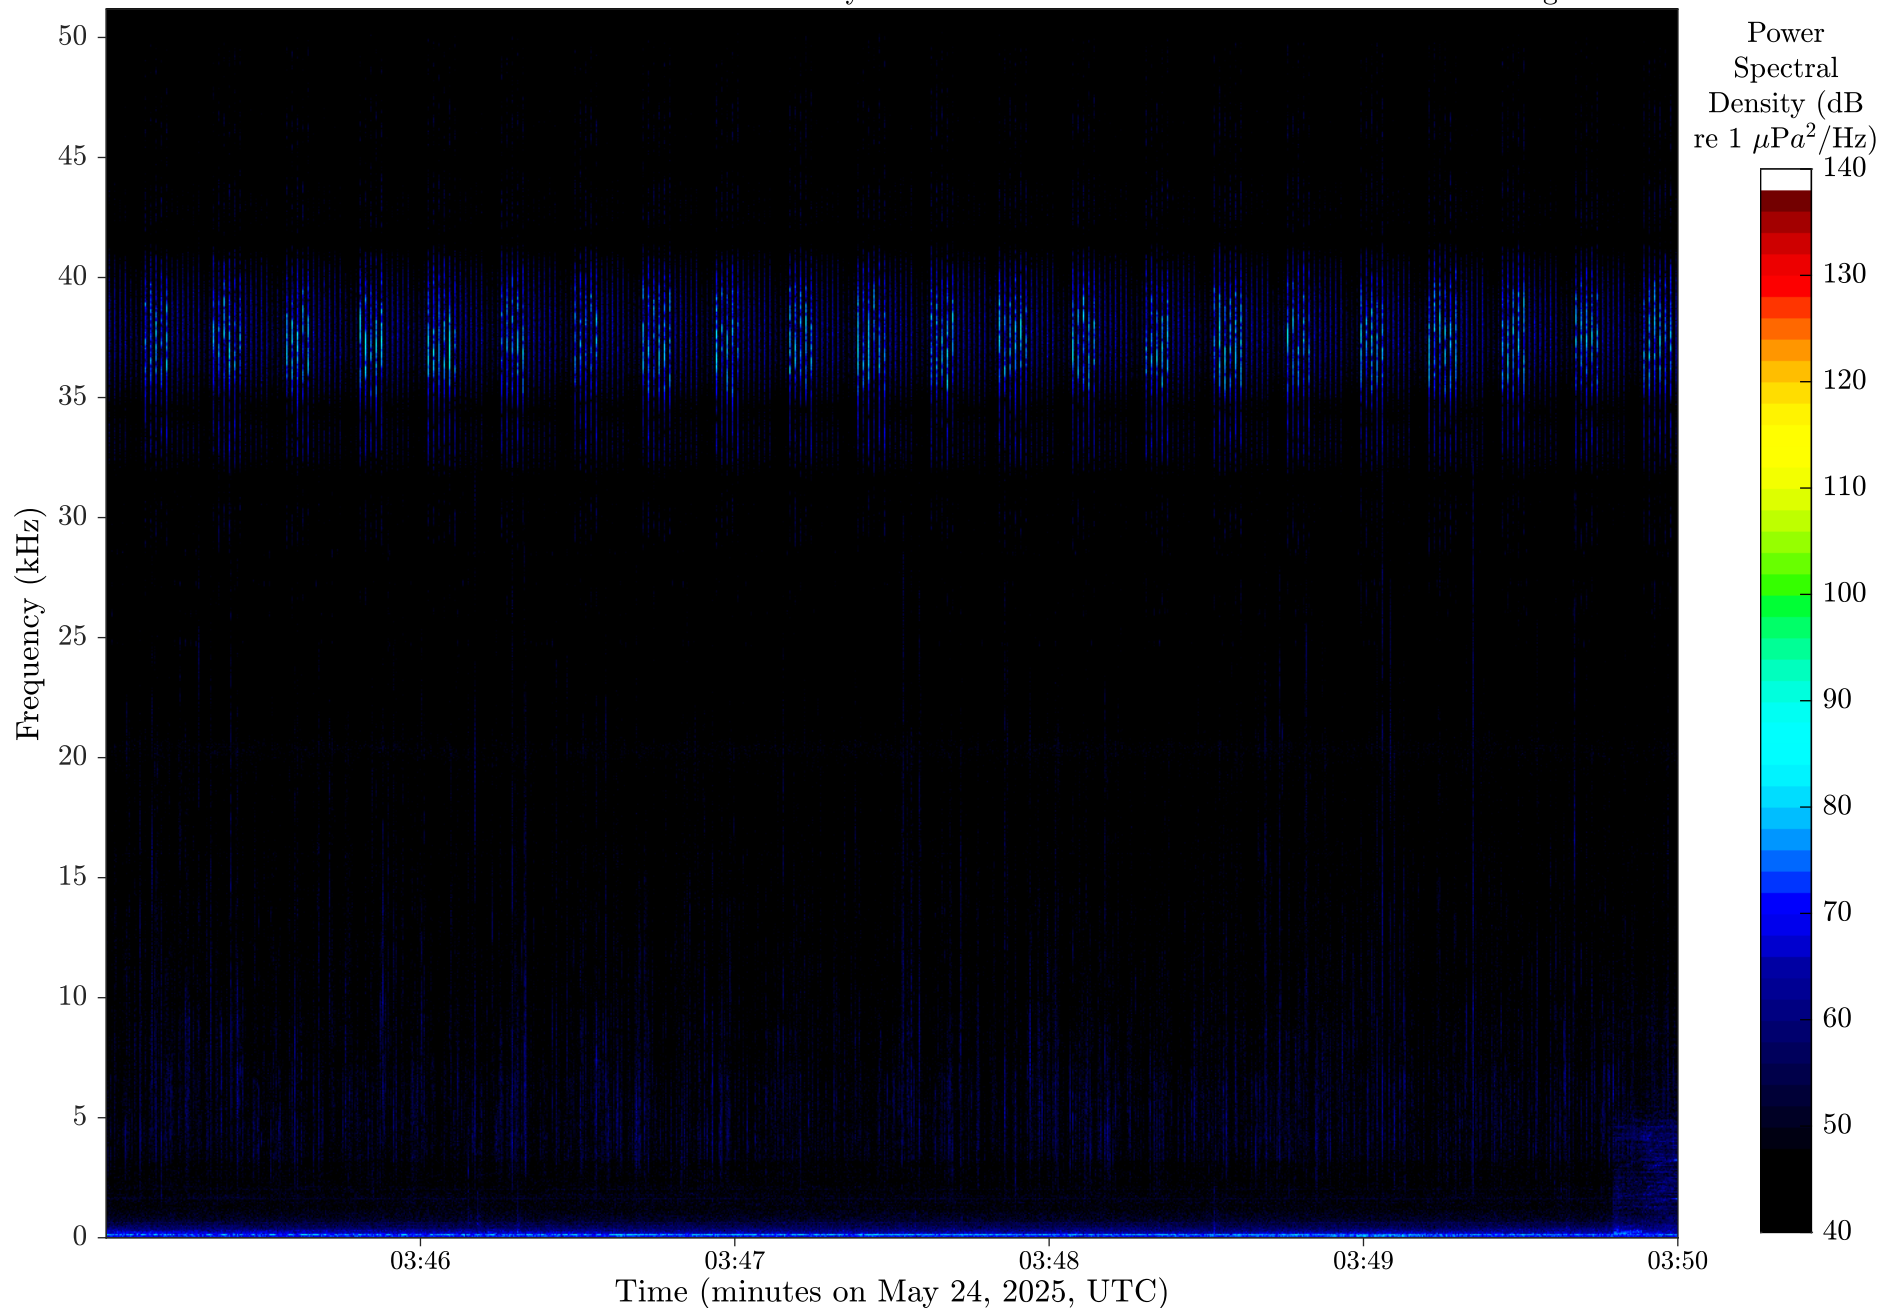


Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:06 UTC

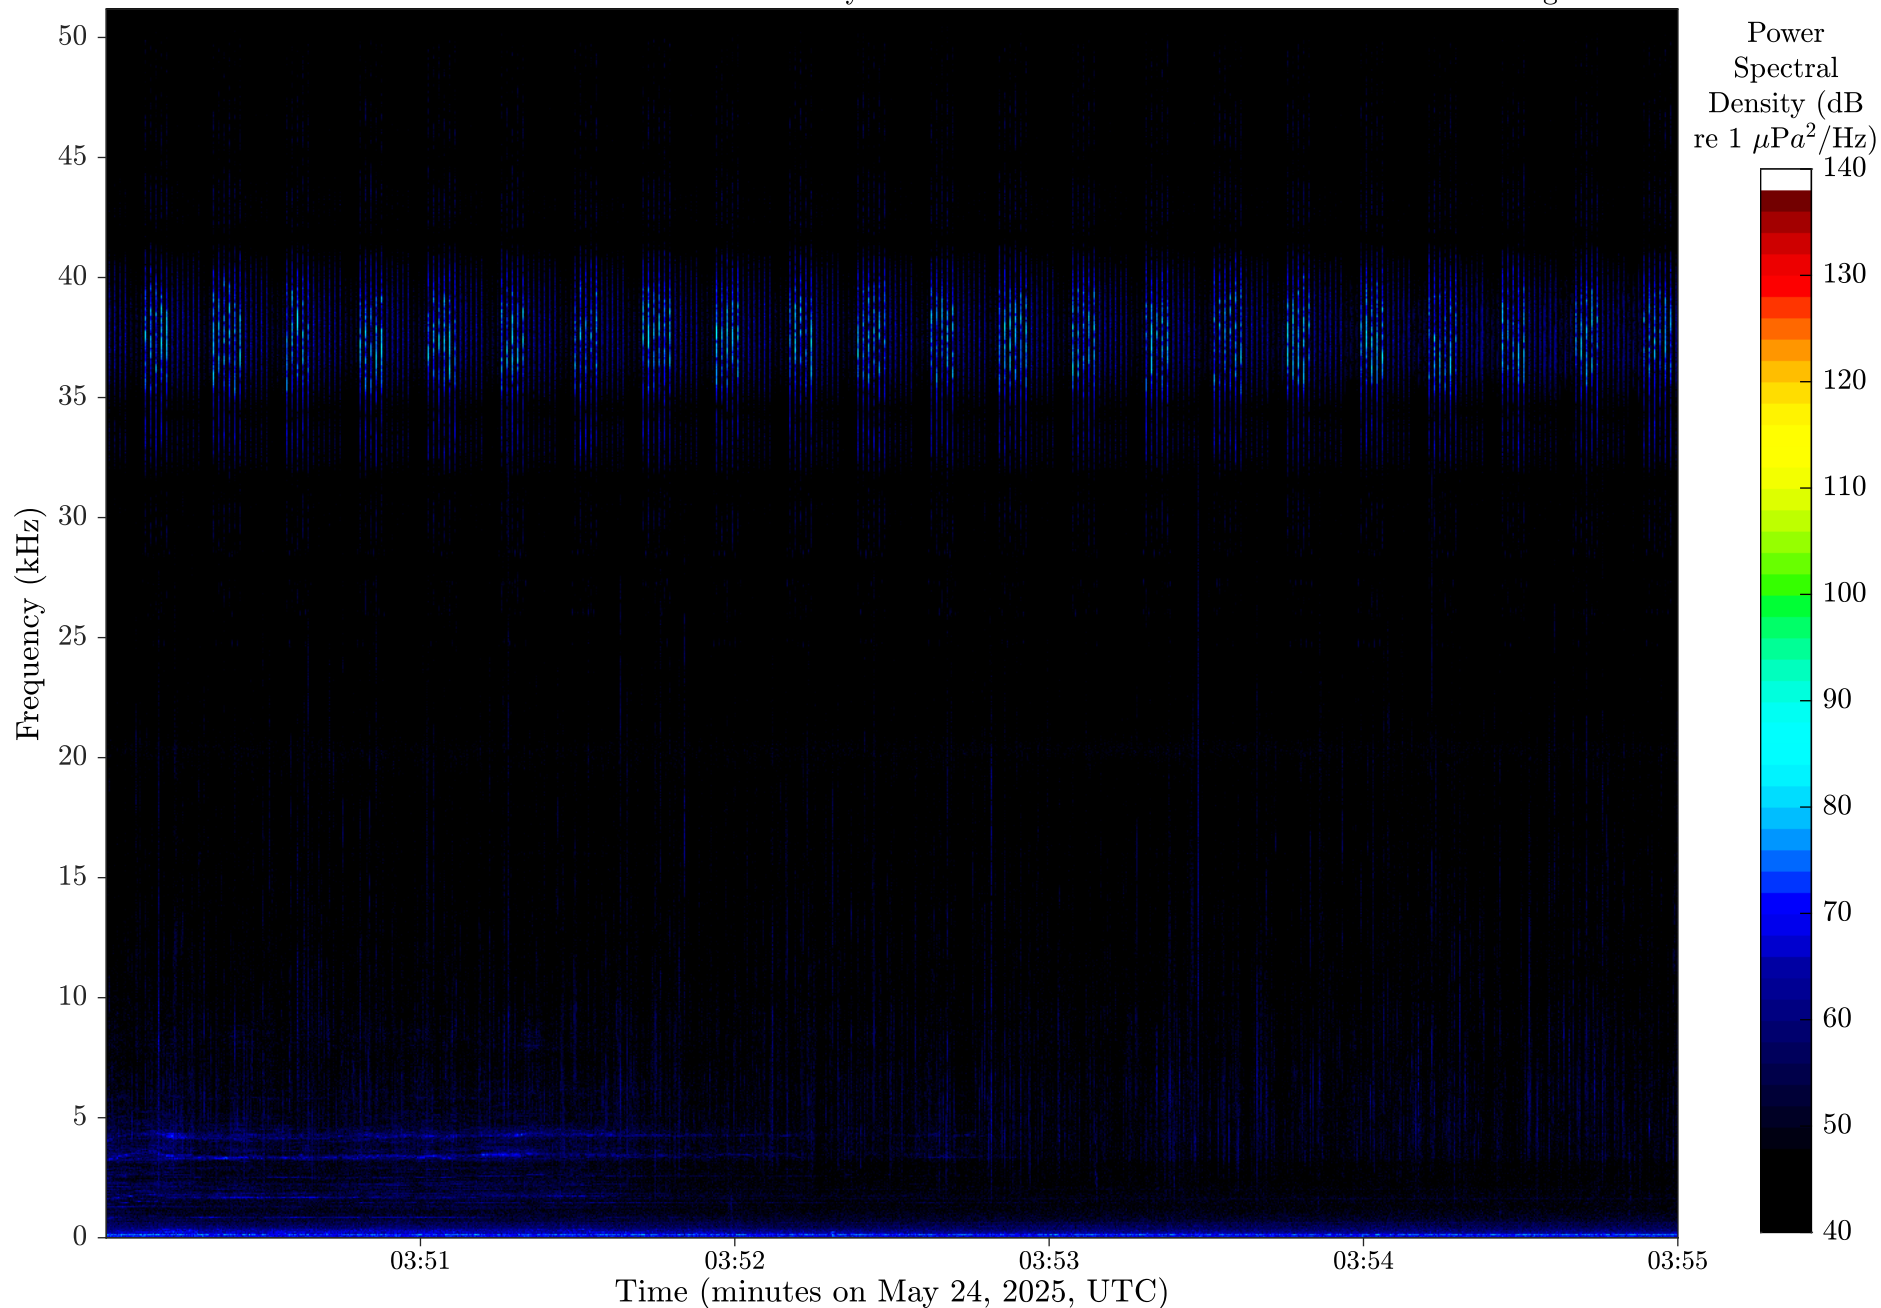


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:14 UTC

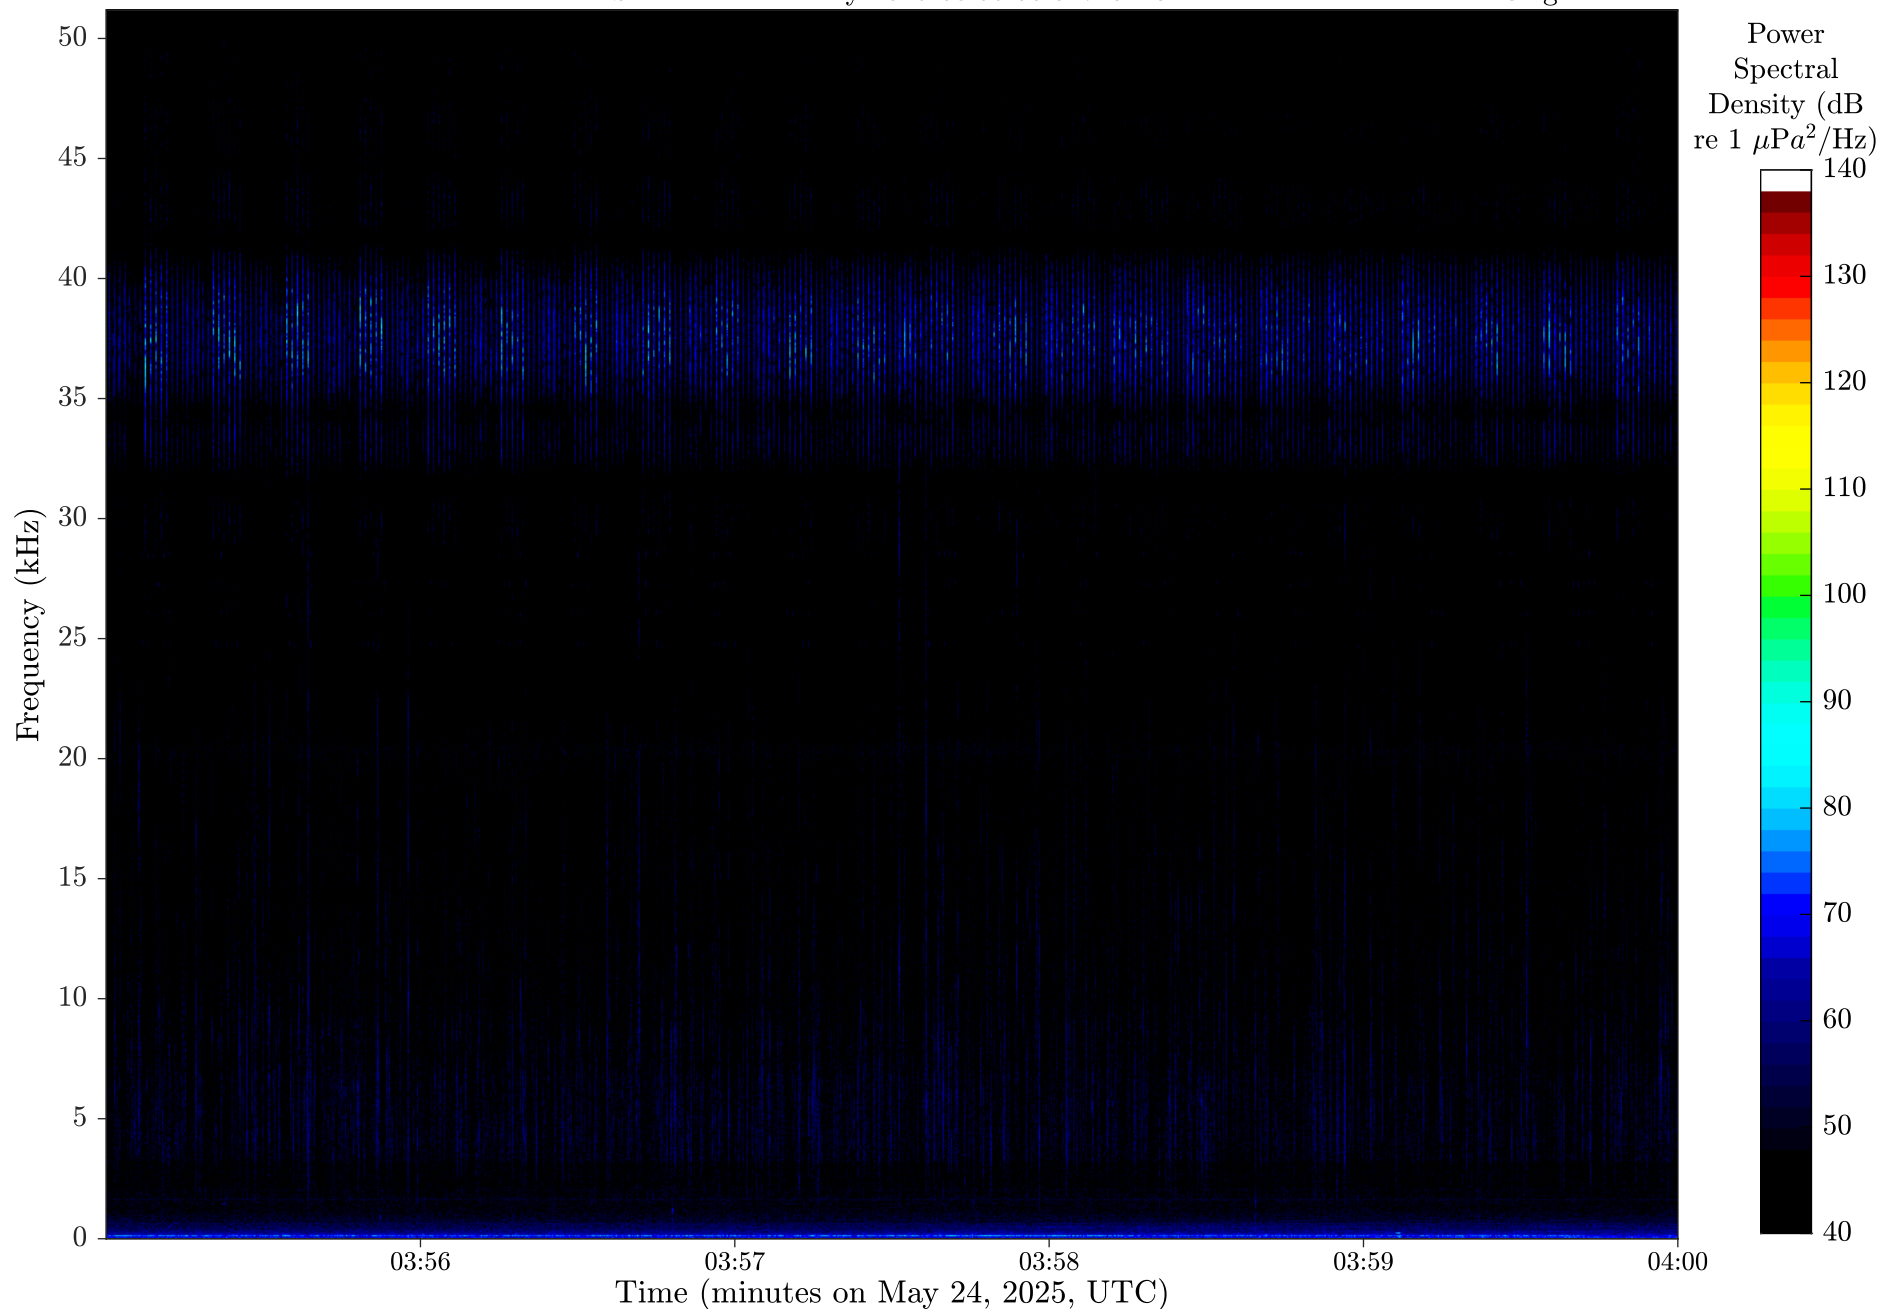


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:22 UTC

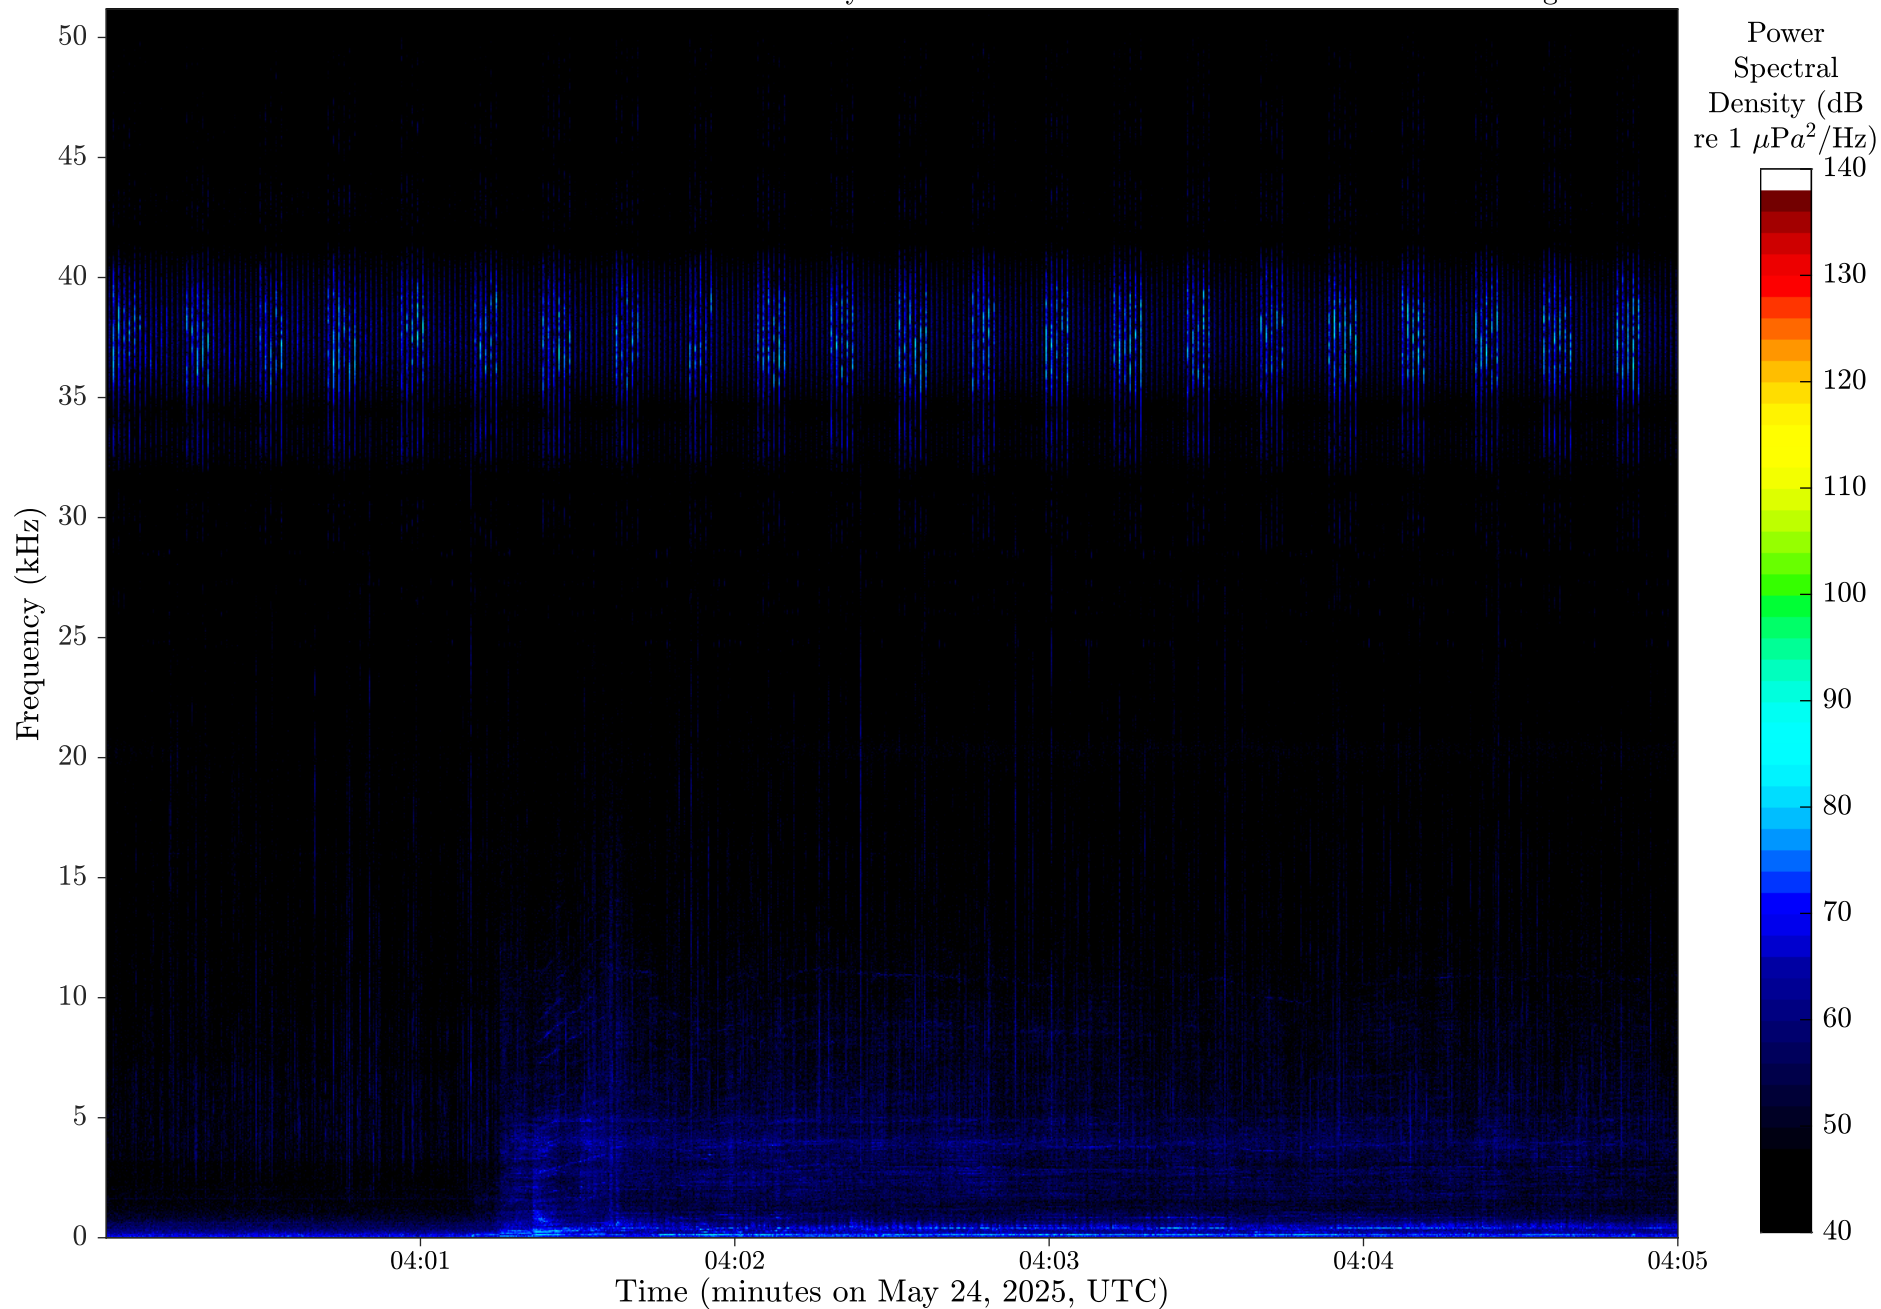


Comments: 32.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:30 UTC

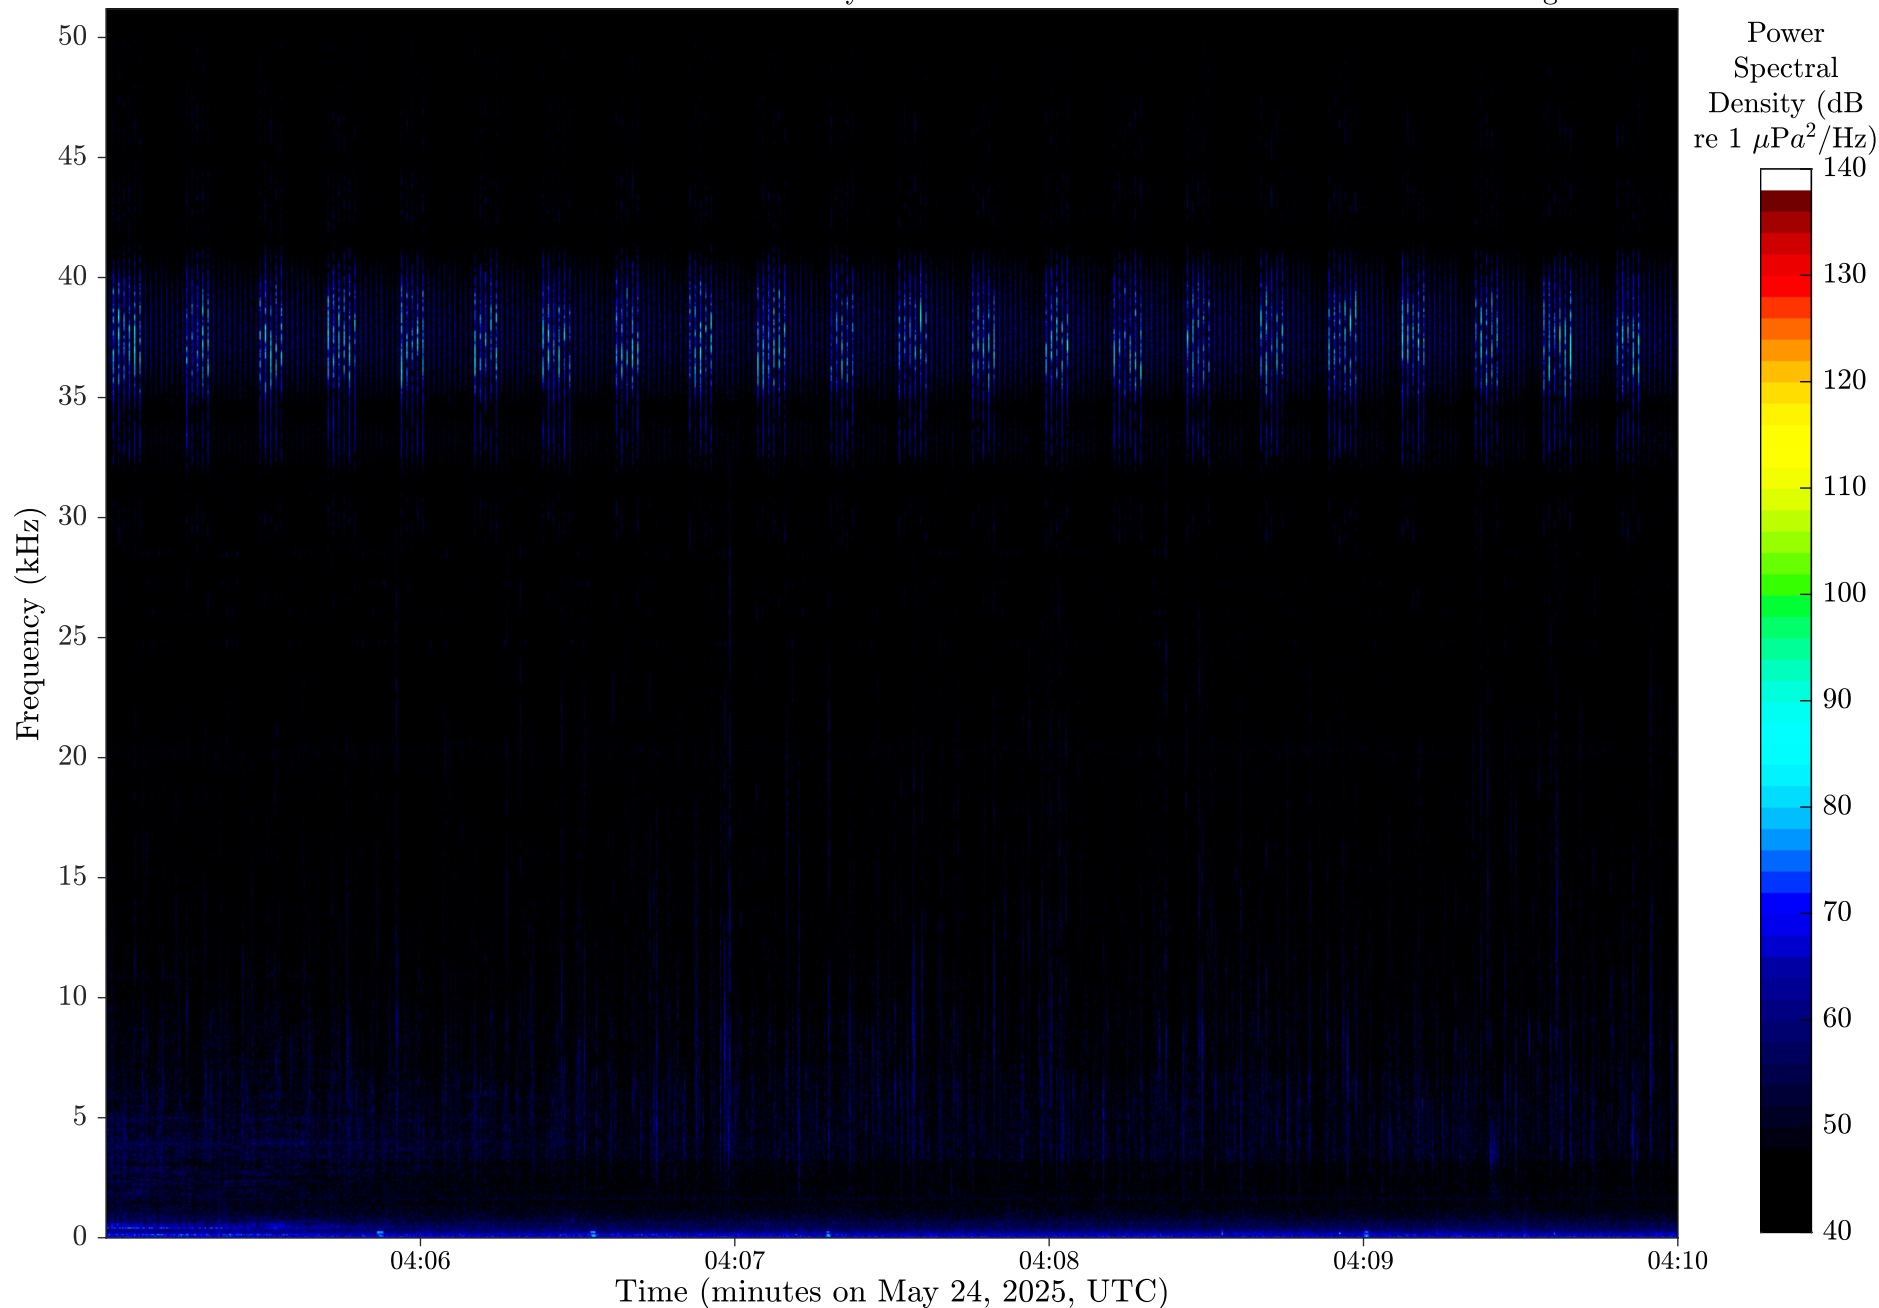


Comments: 34.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:21:38 UTC

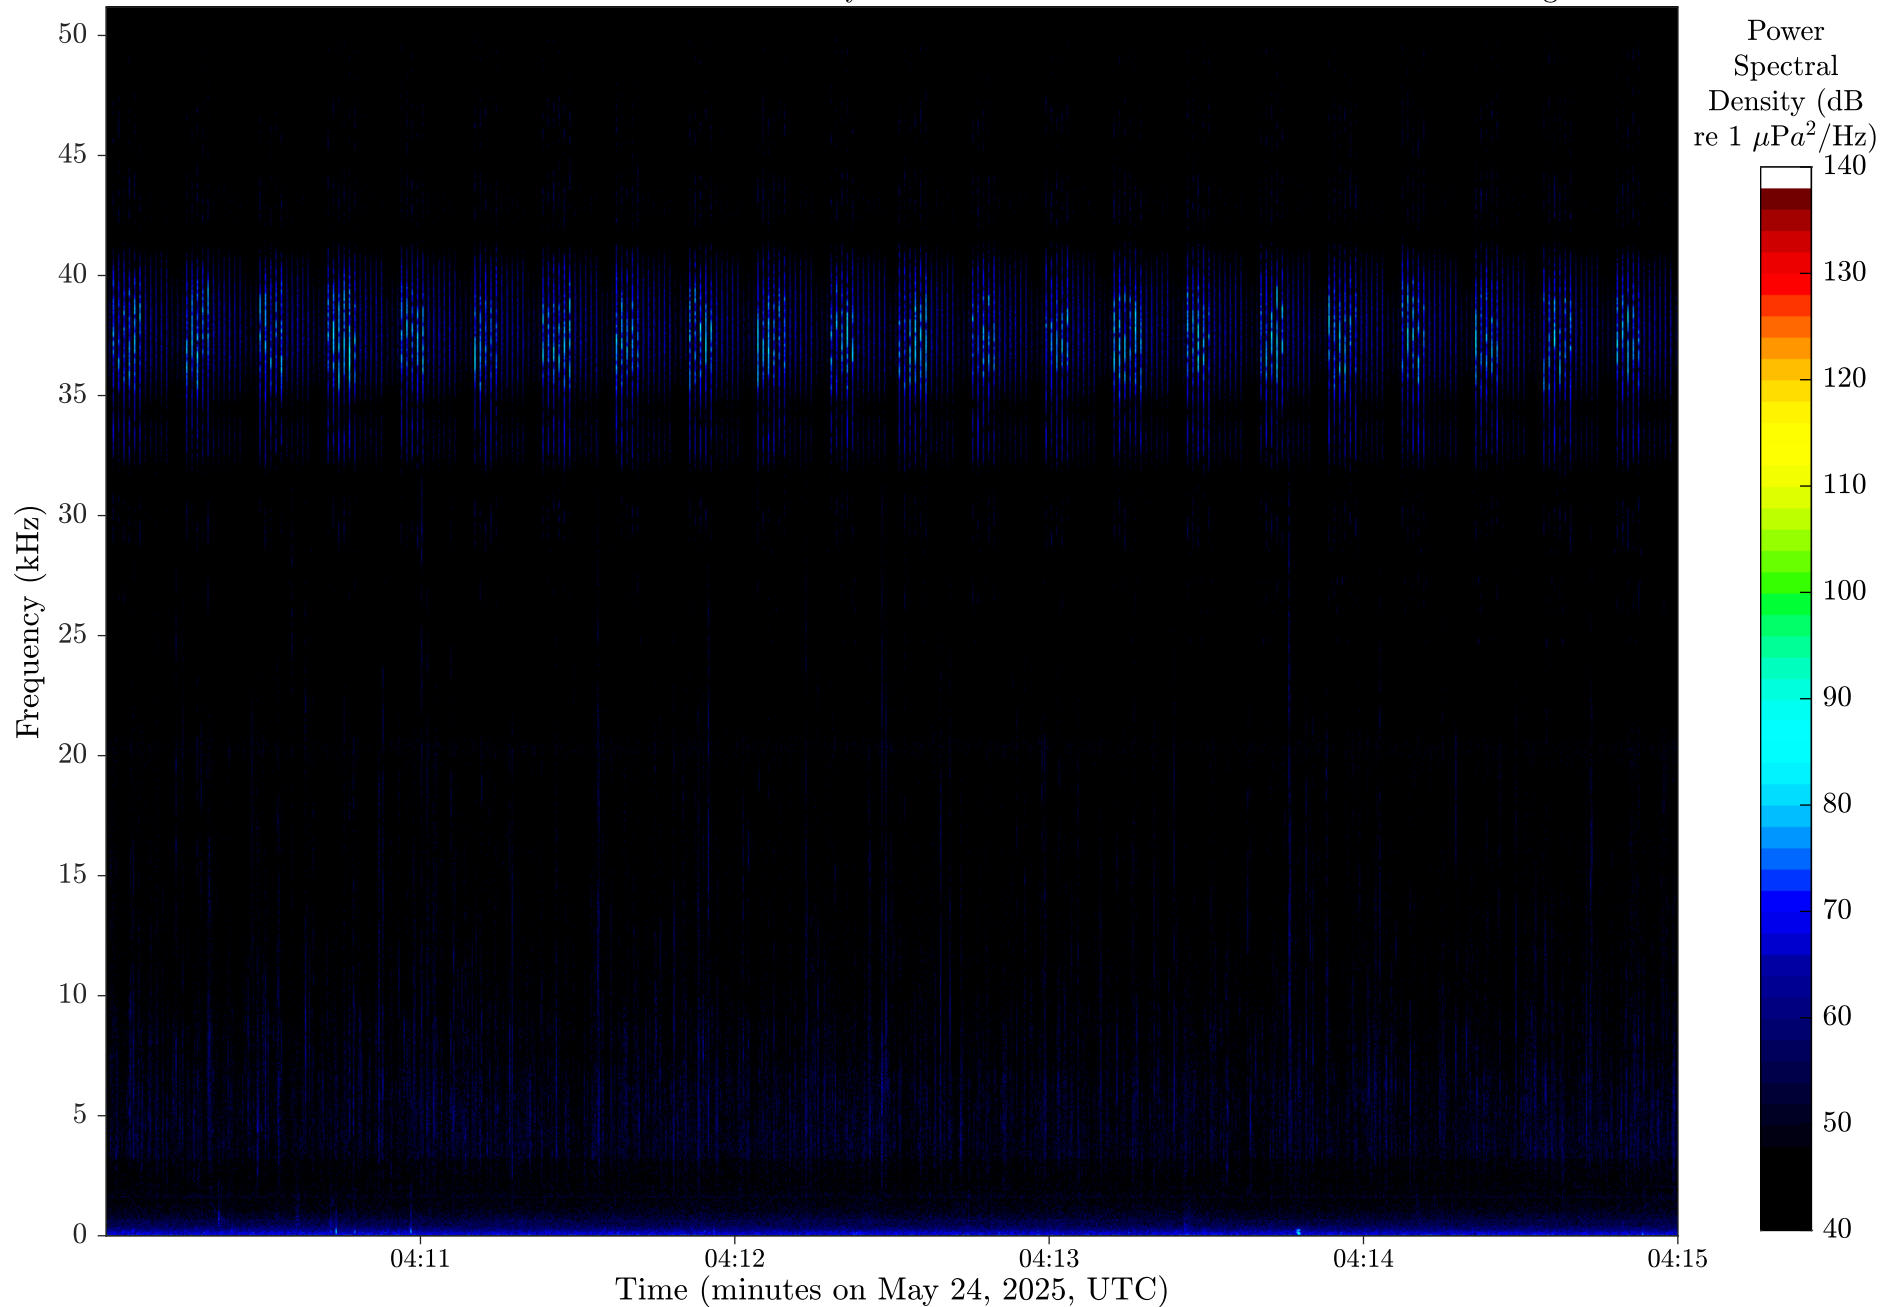


Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:47 UTC

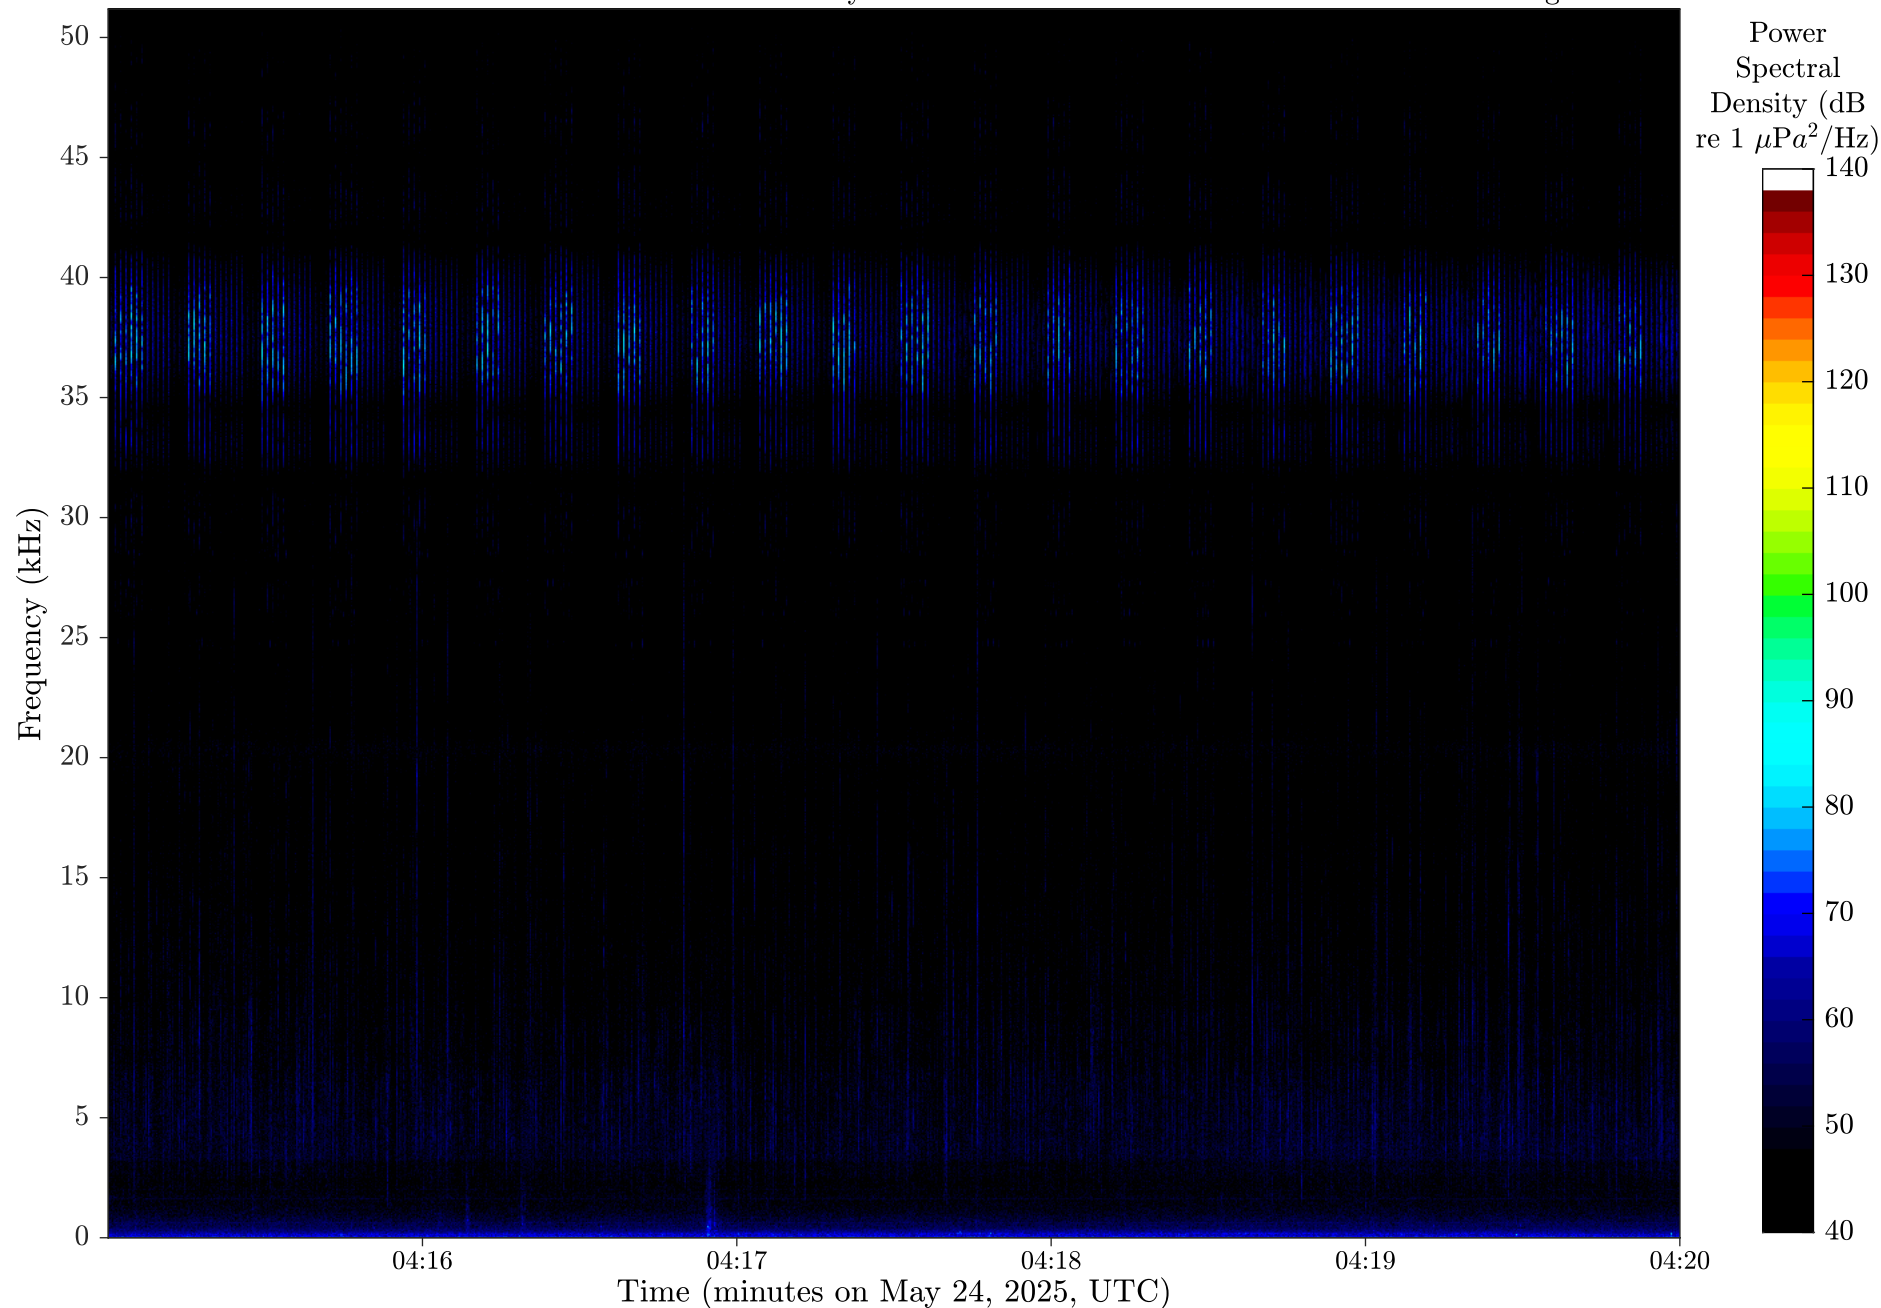


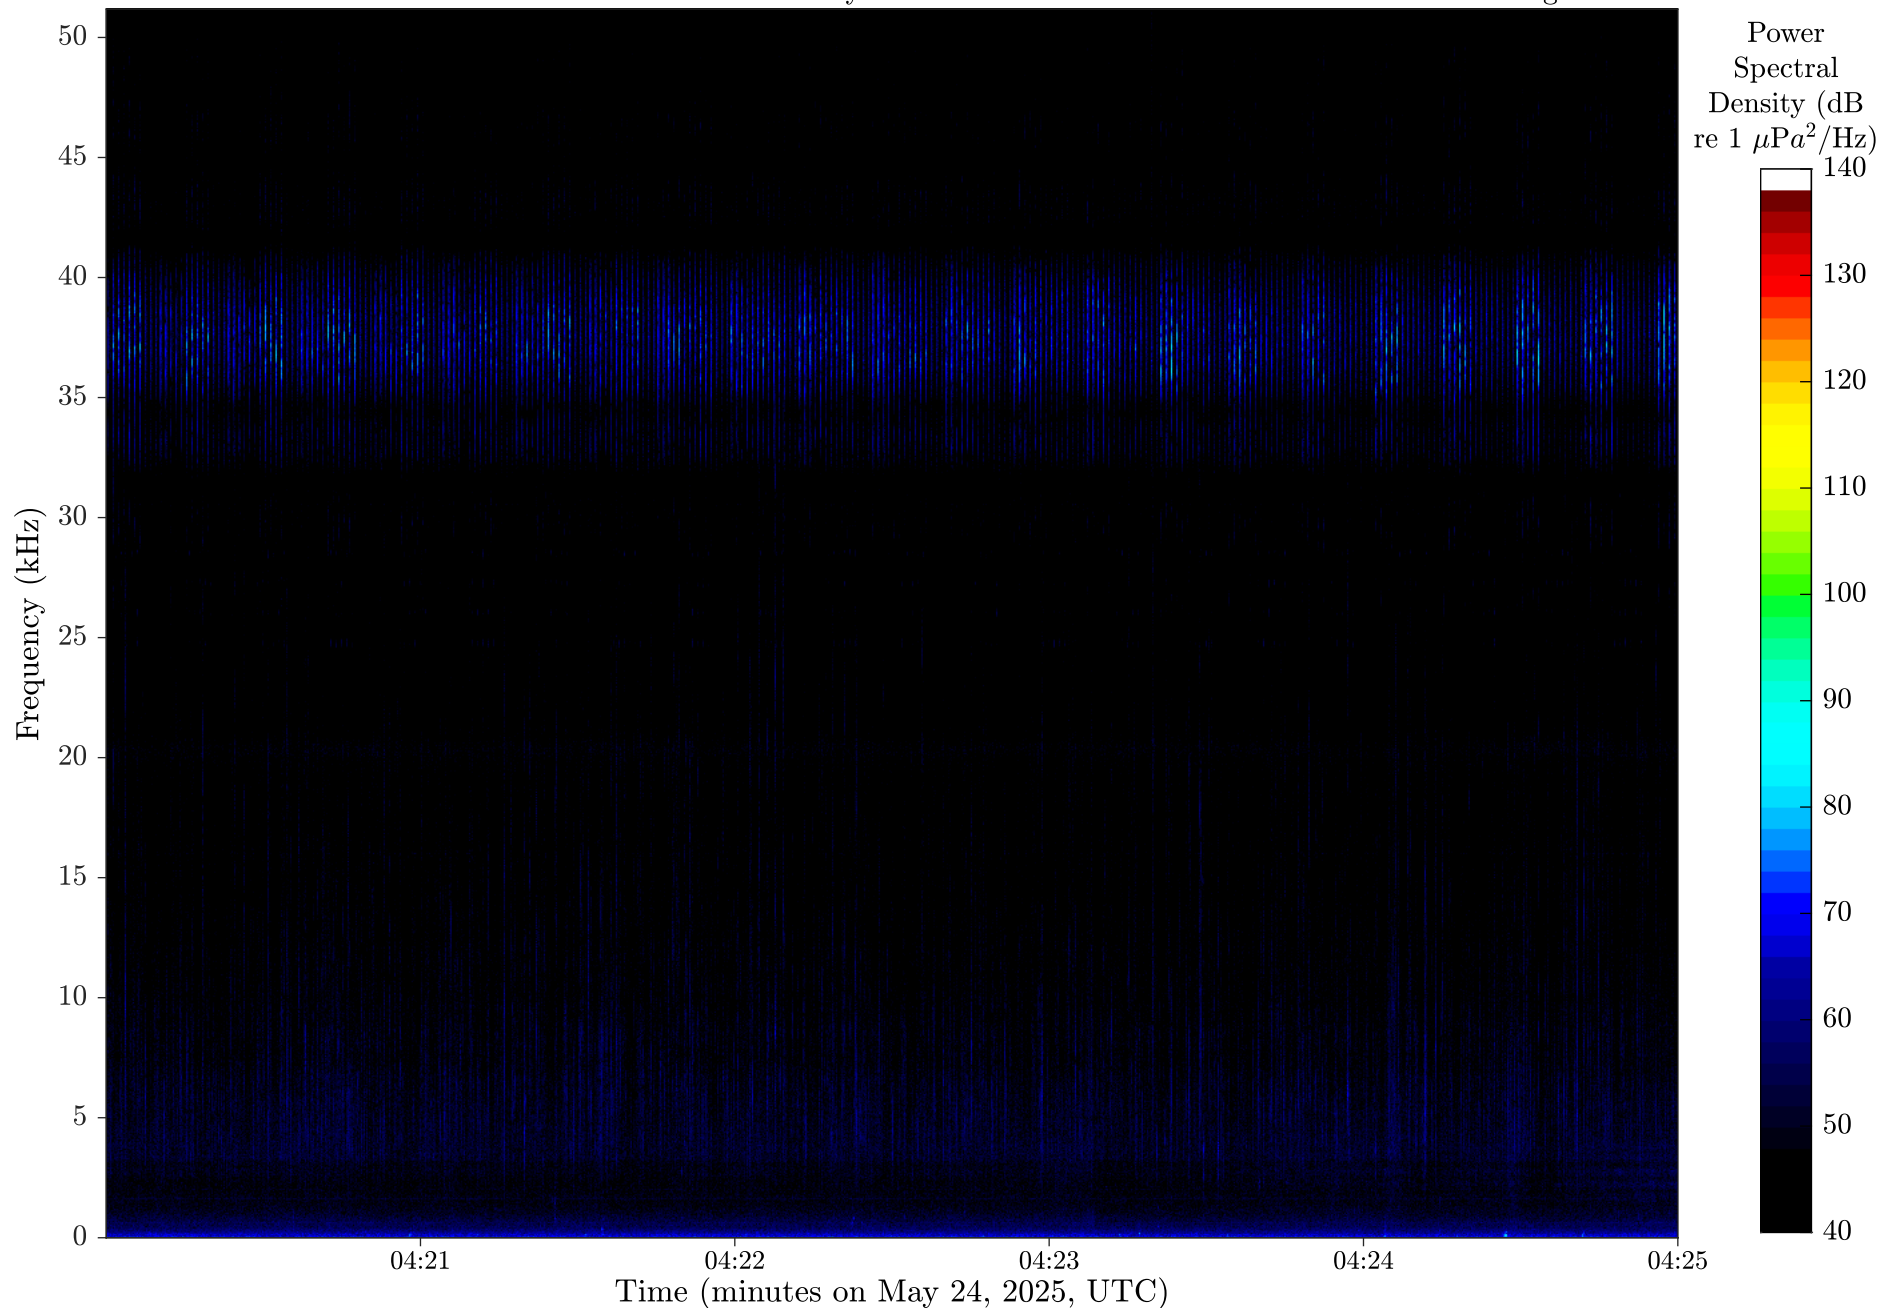


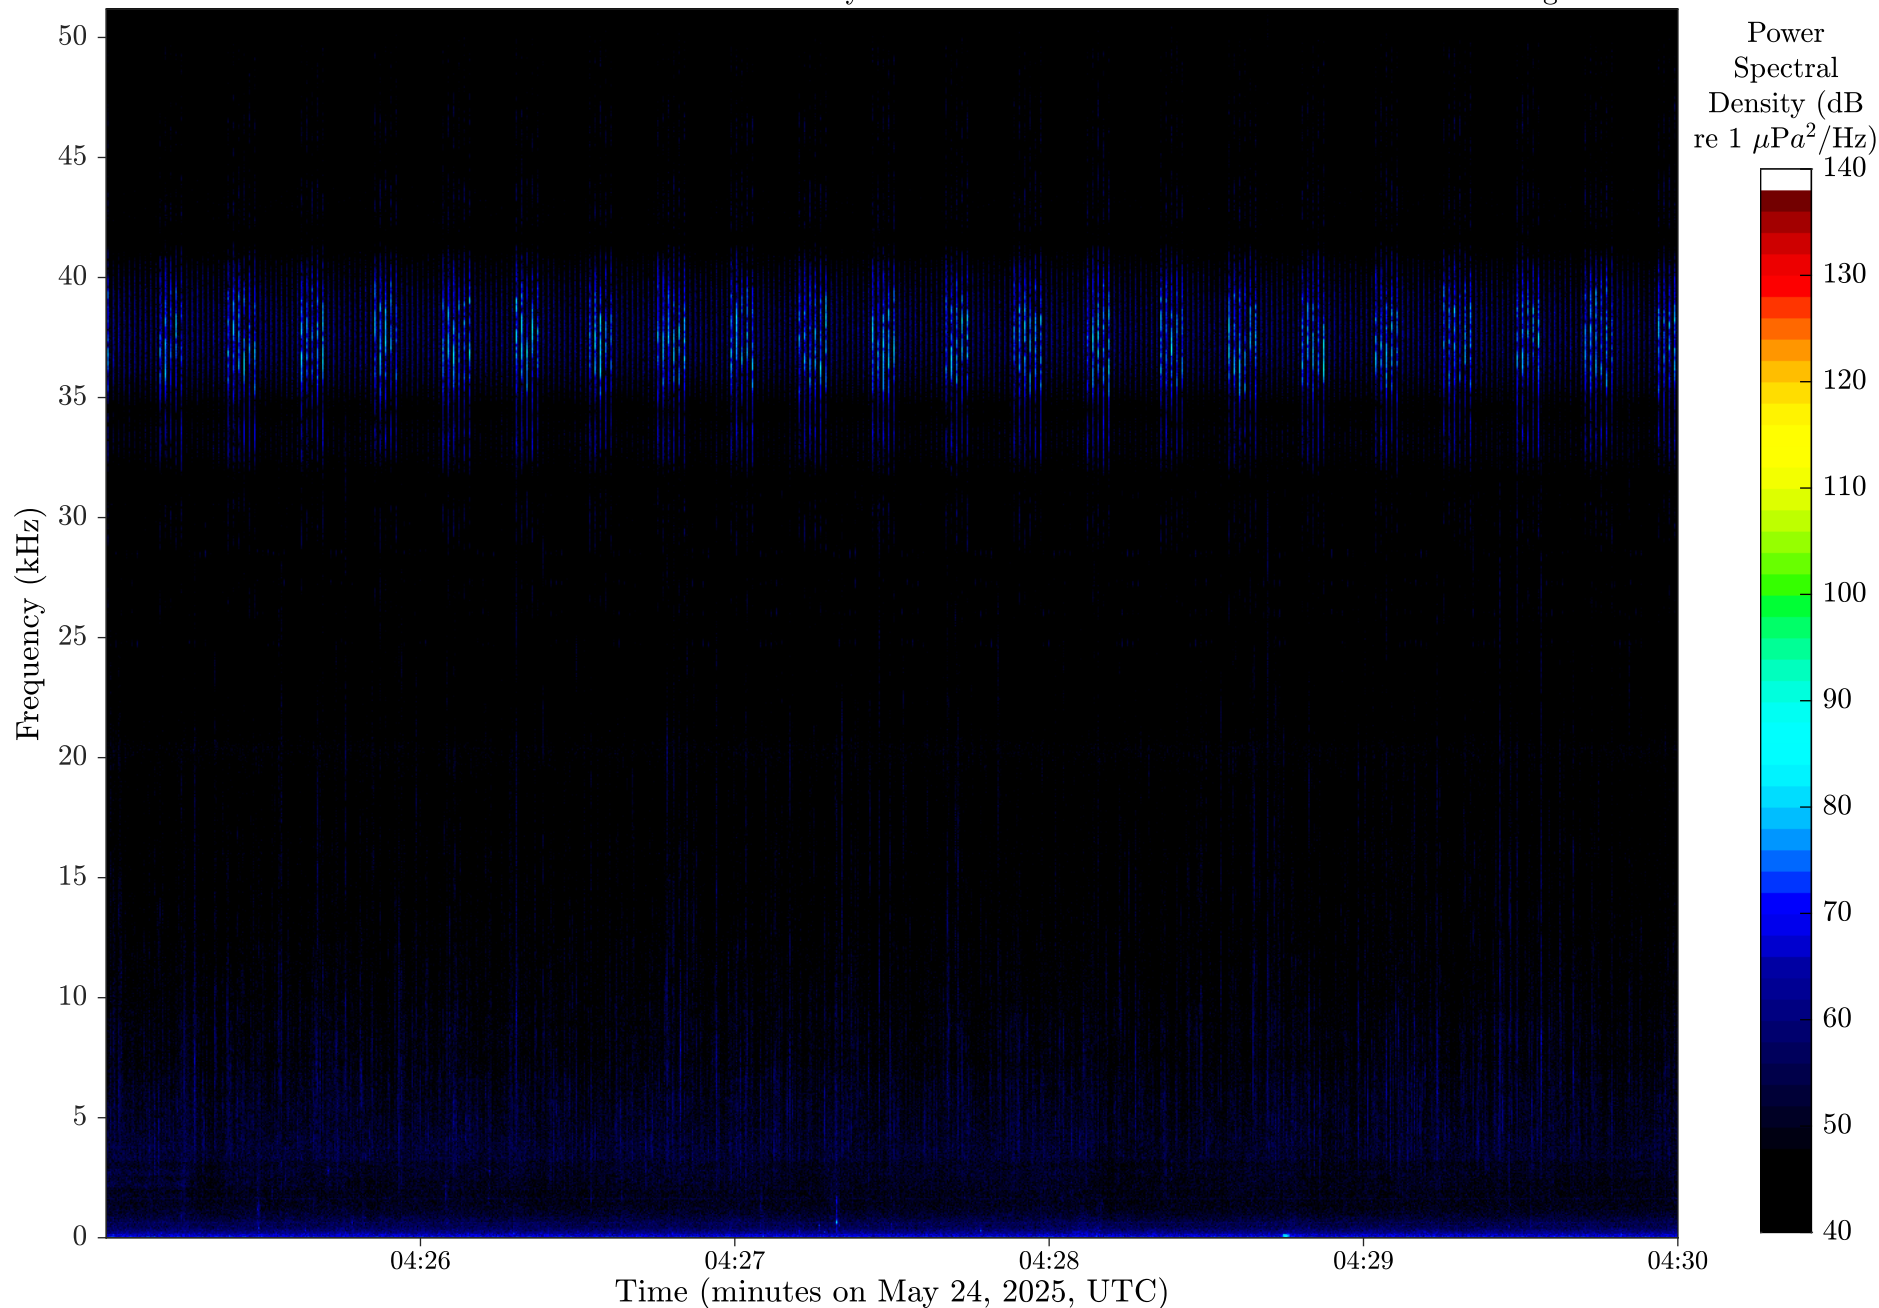

Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:22:12 UTC

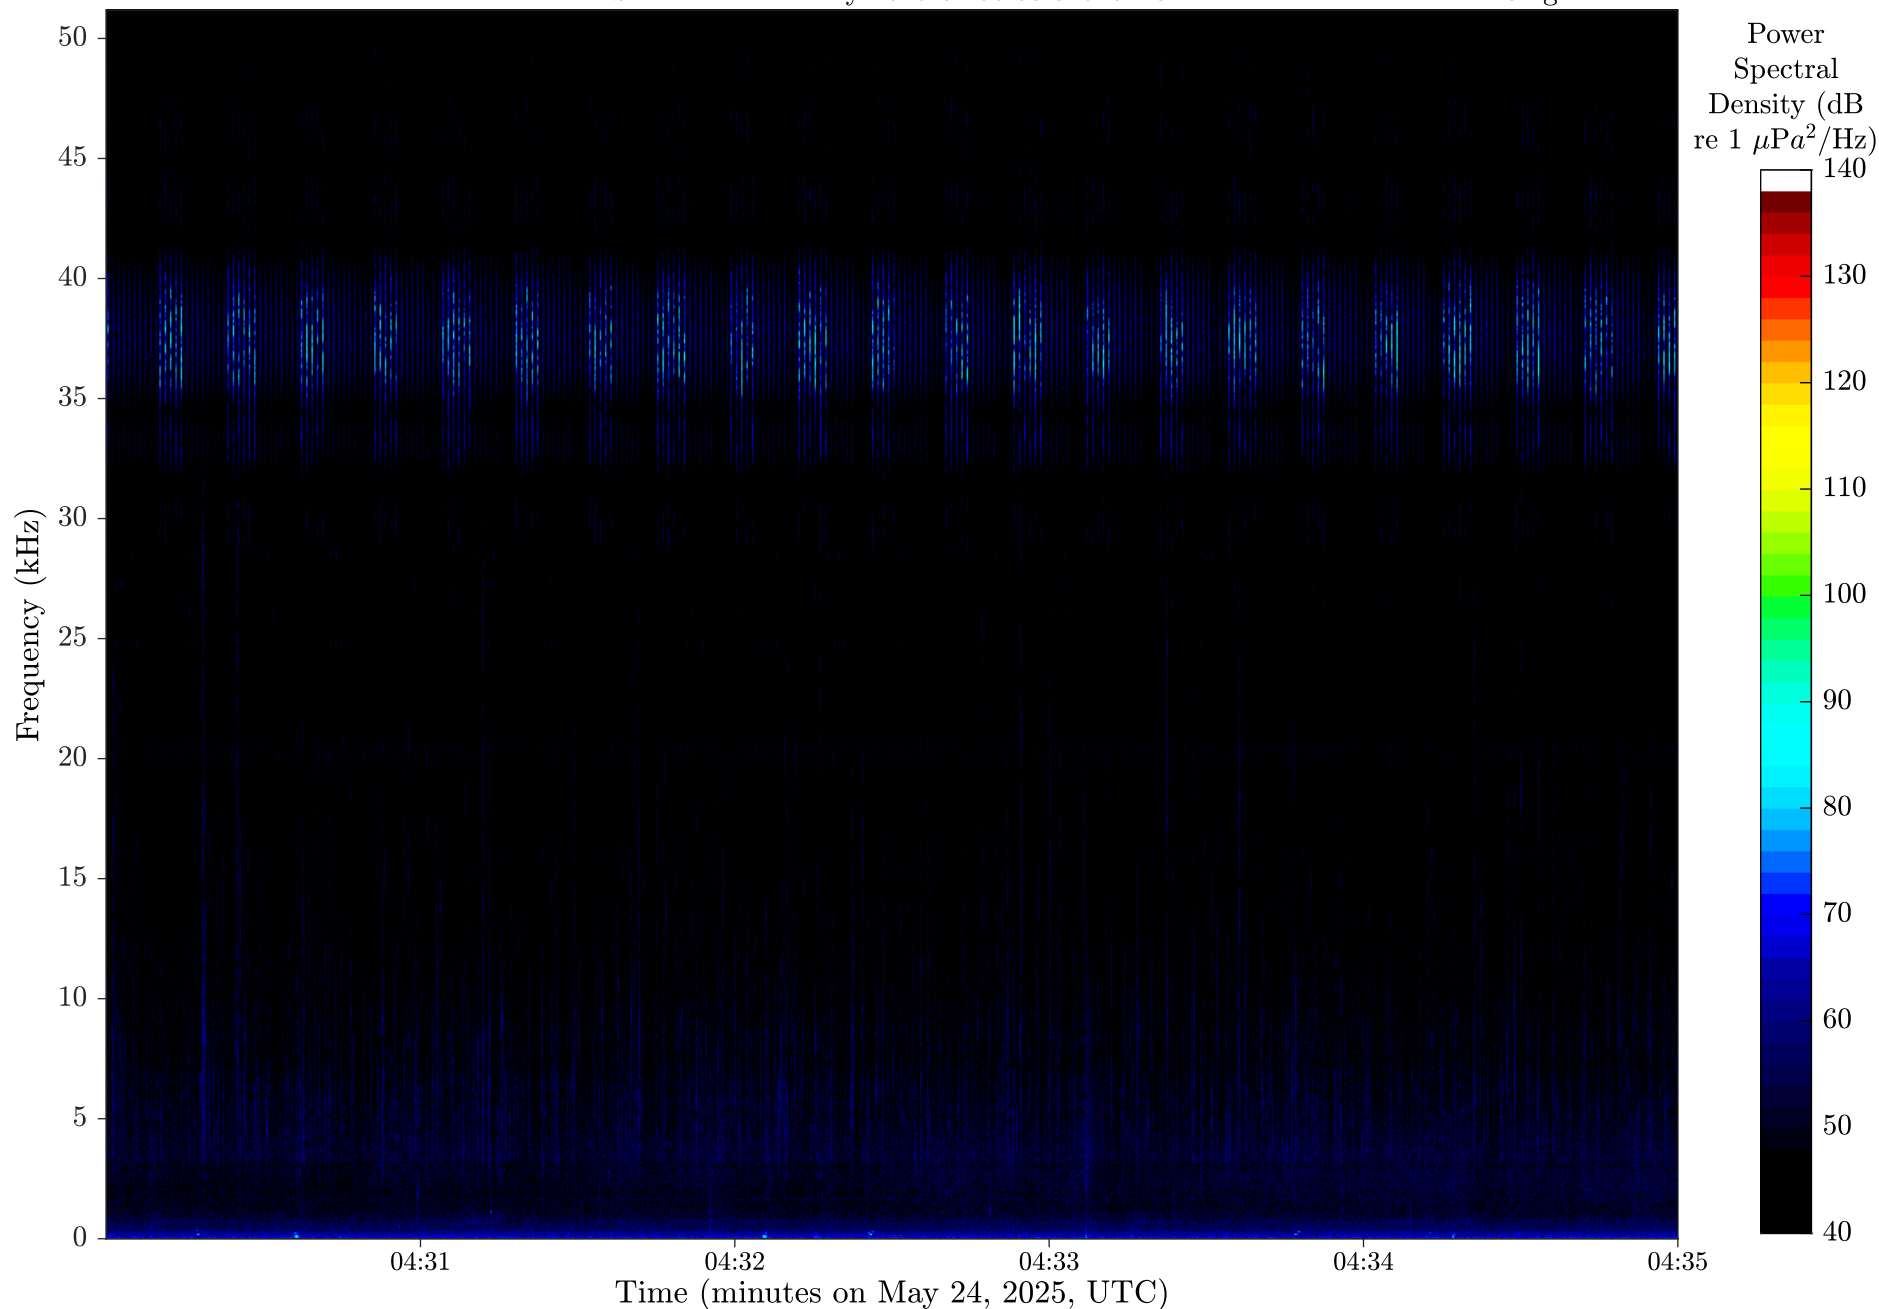

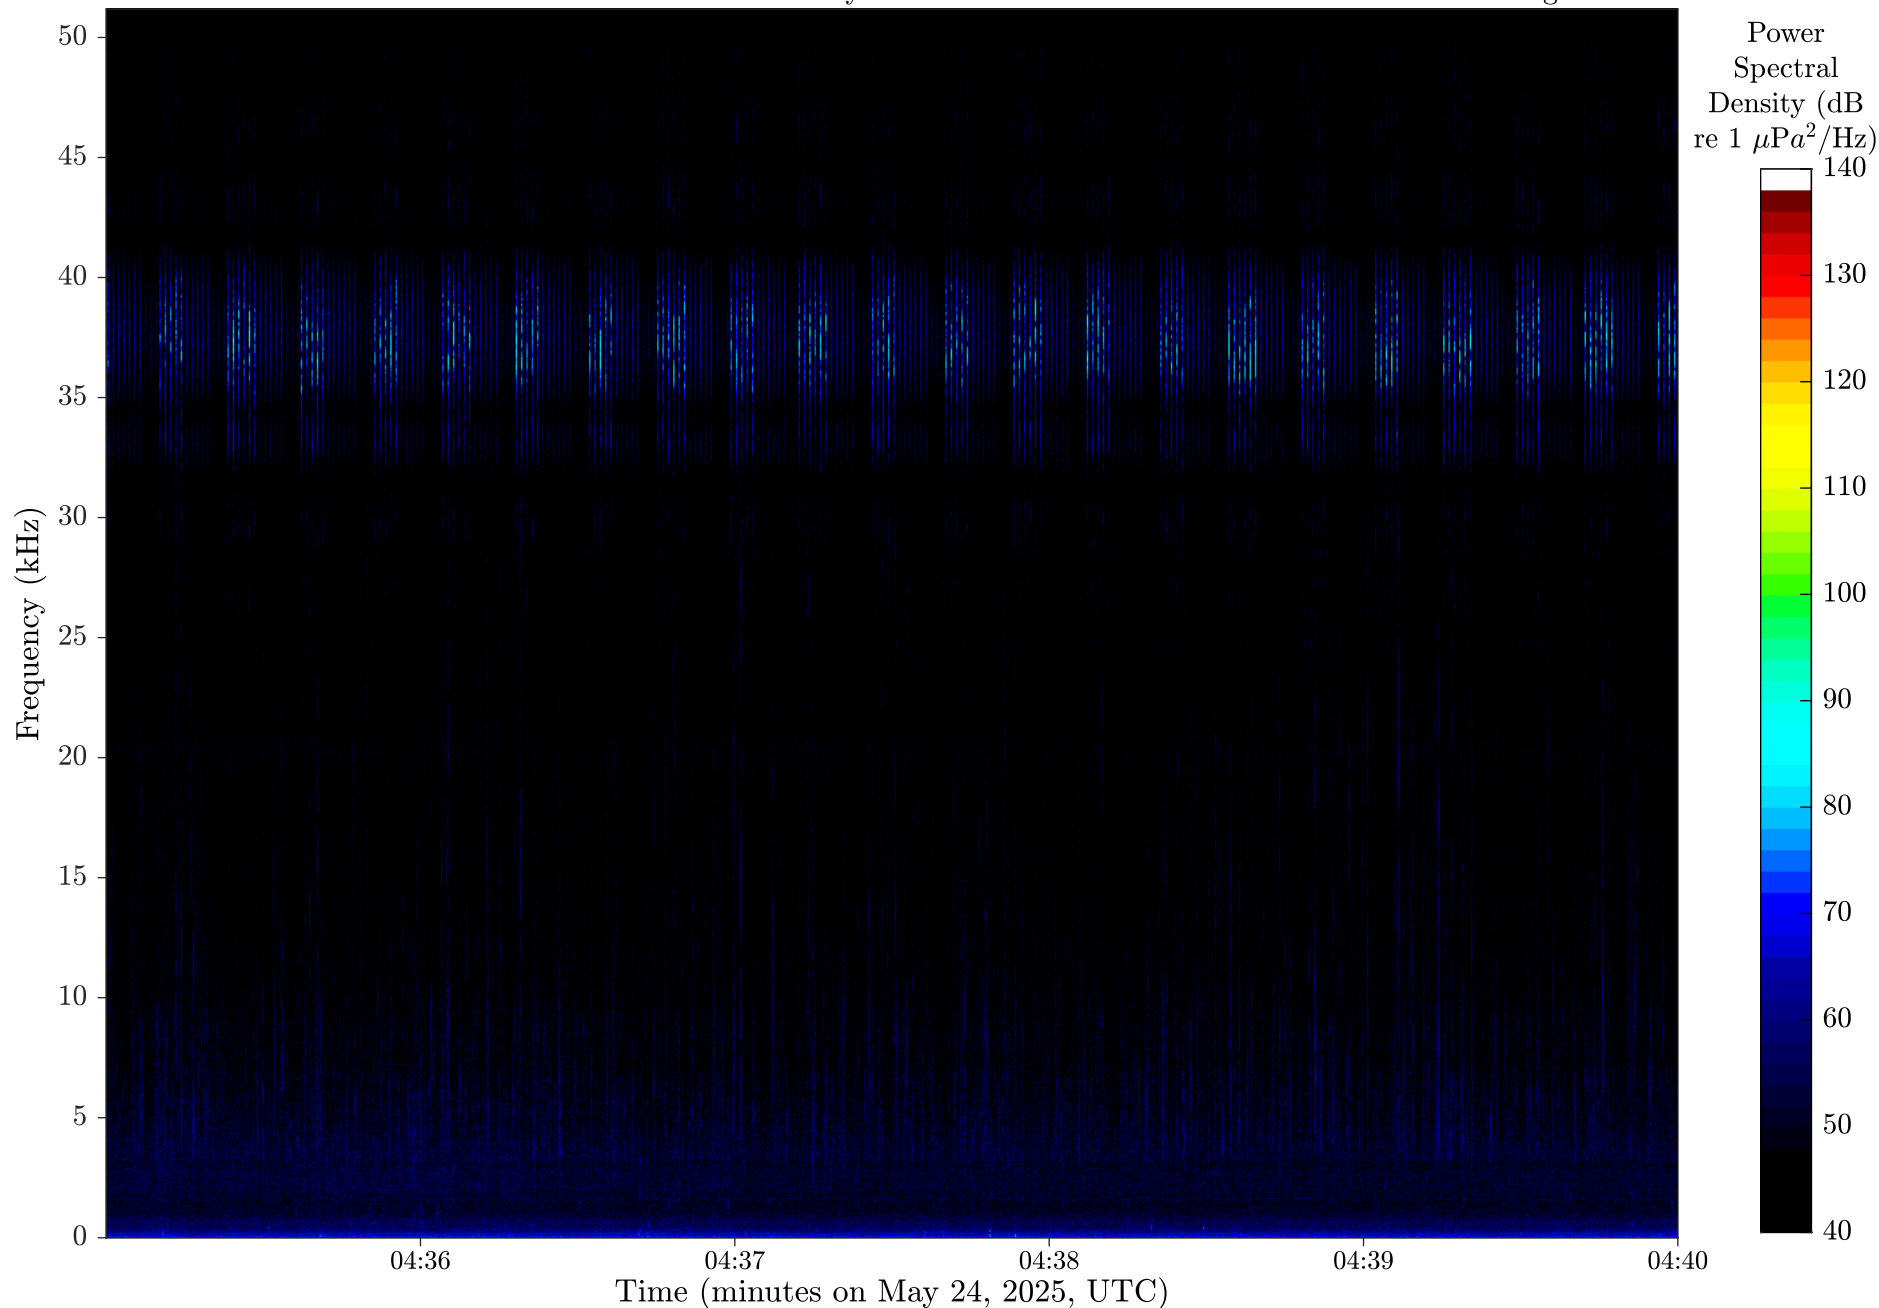


Comments: 34.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:29 UTC

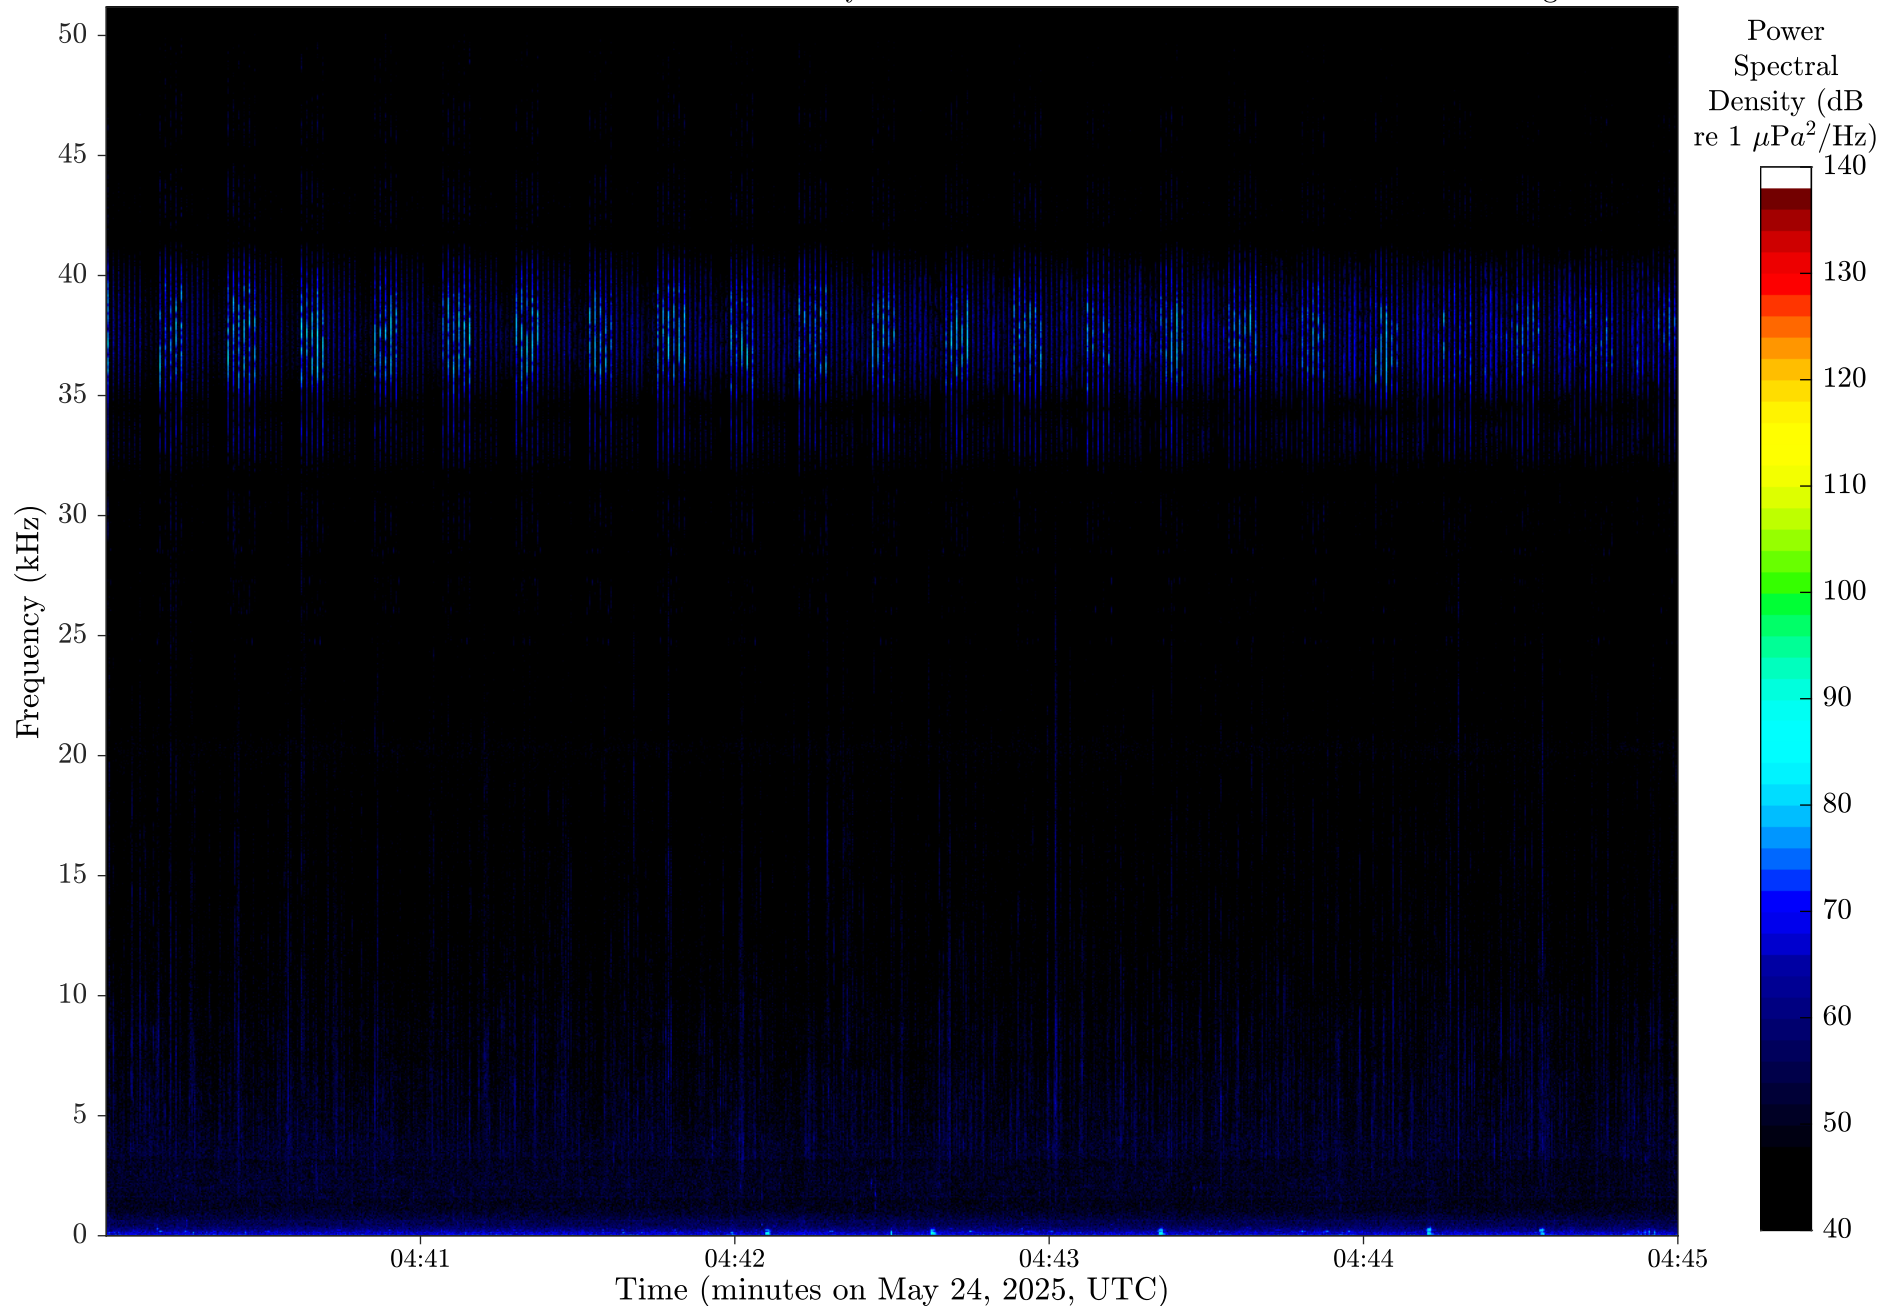


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:38 UTC

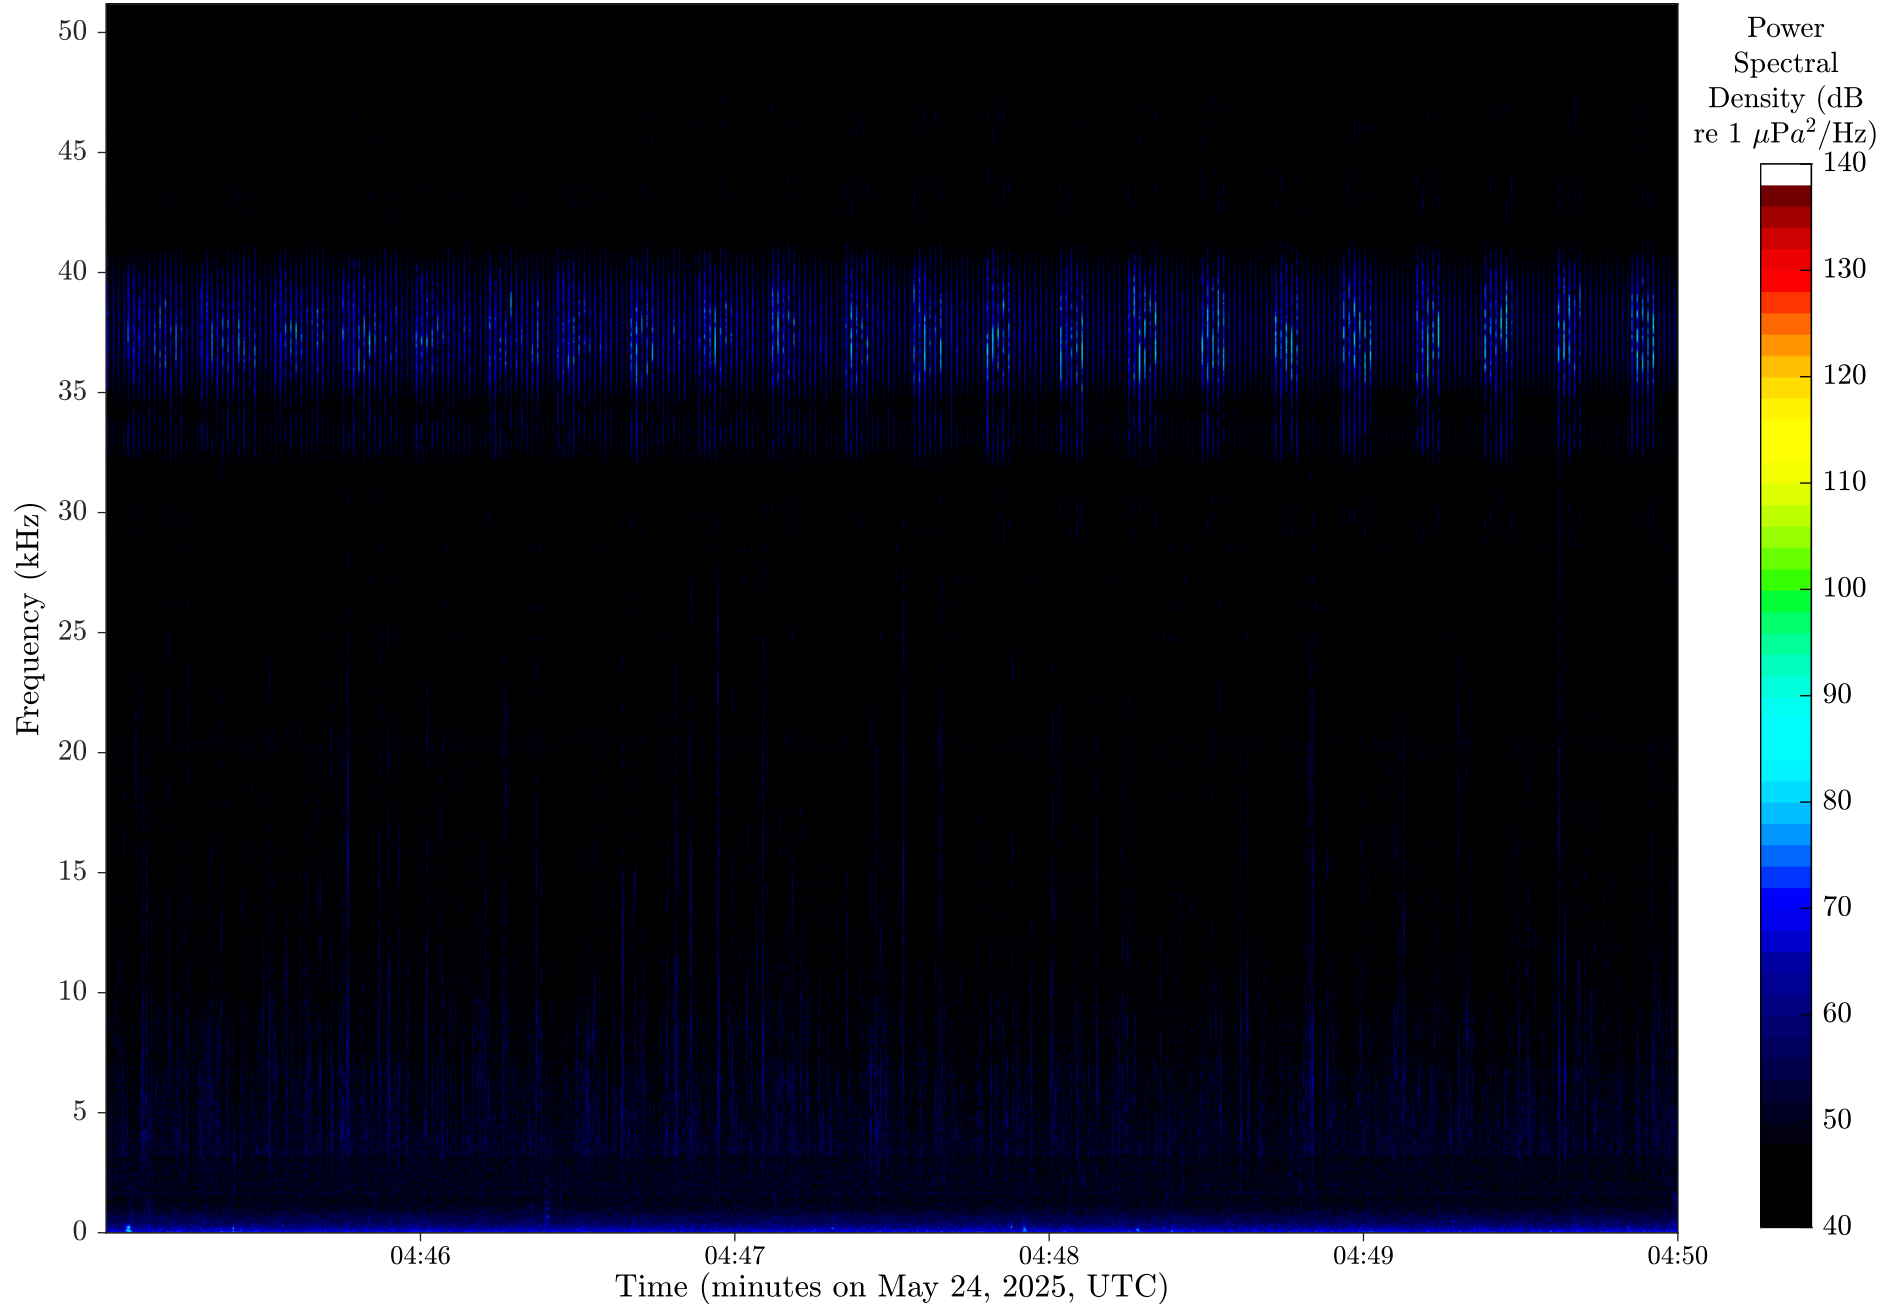


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:46 UTC

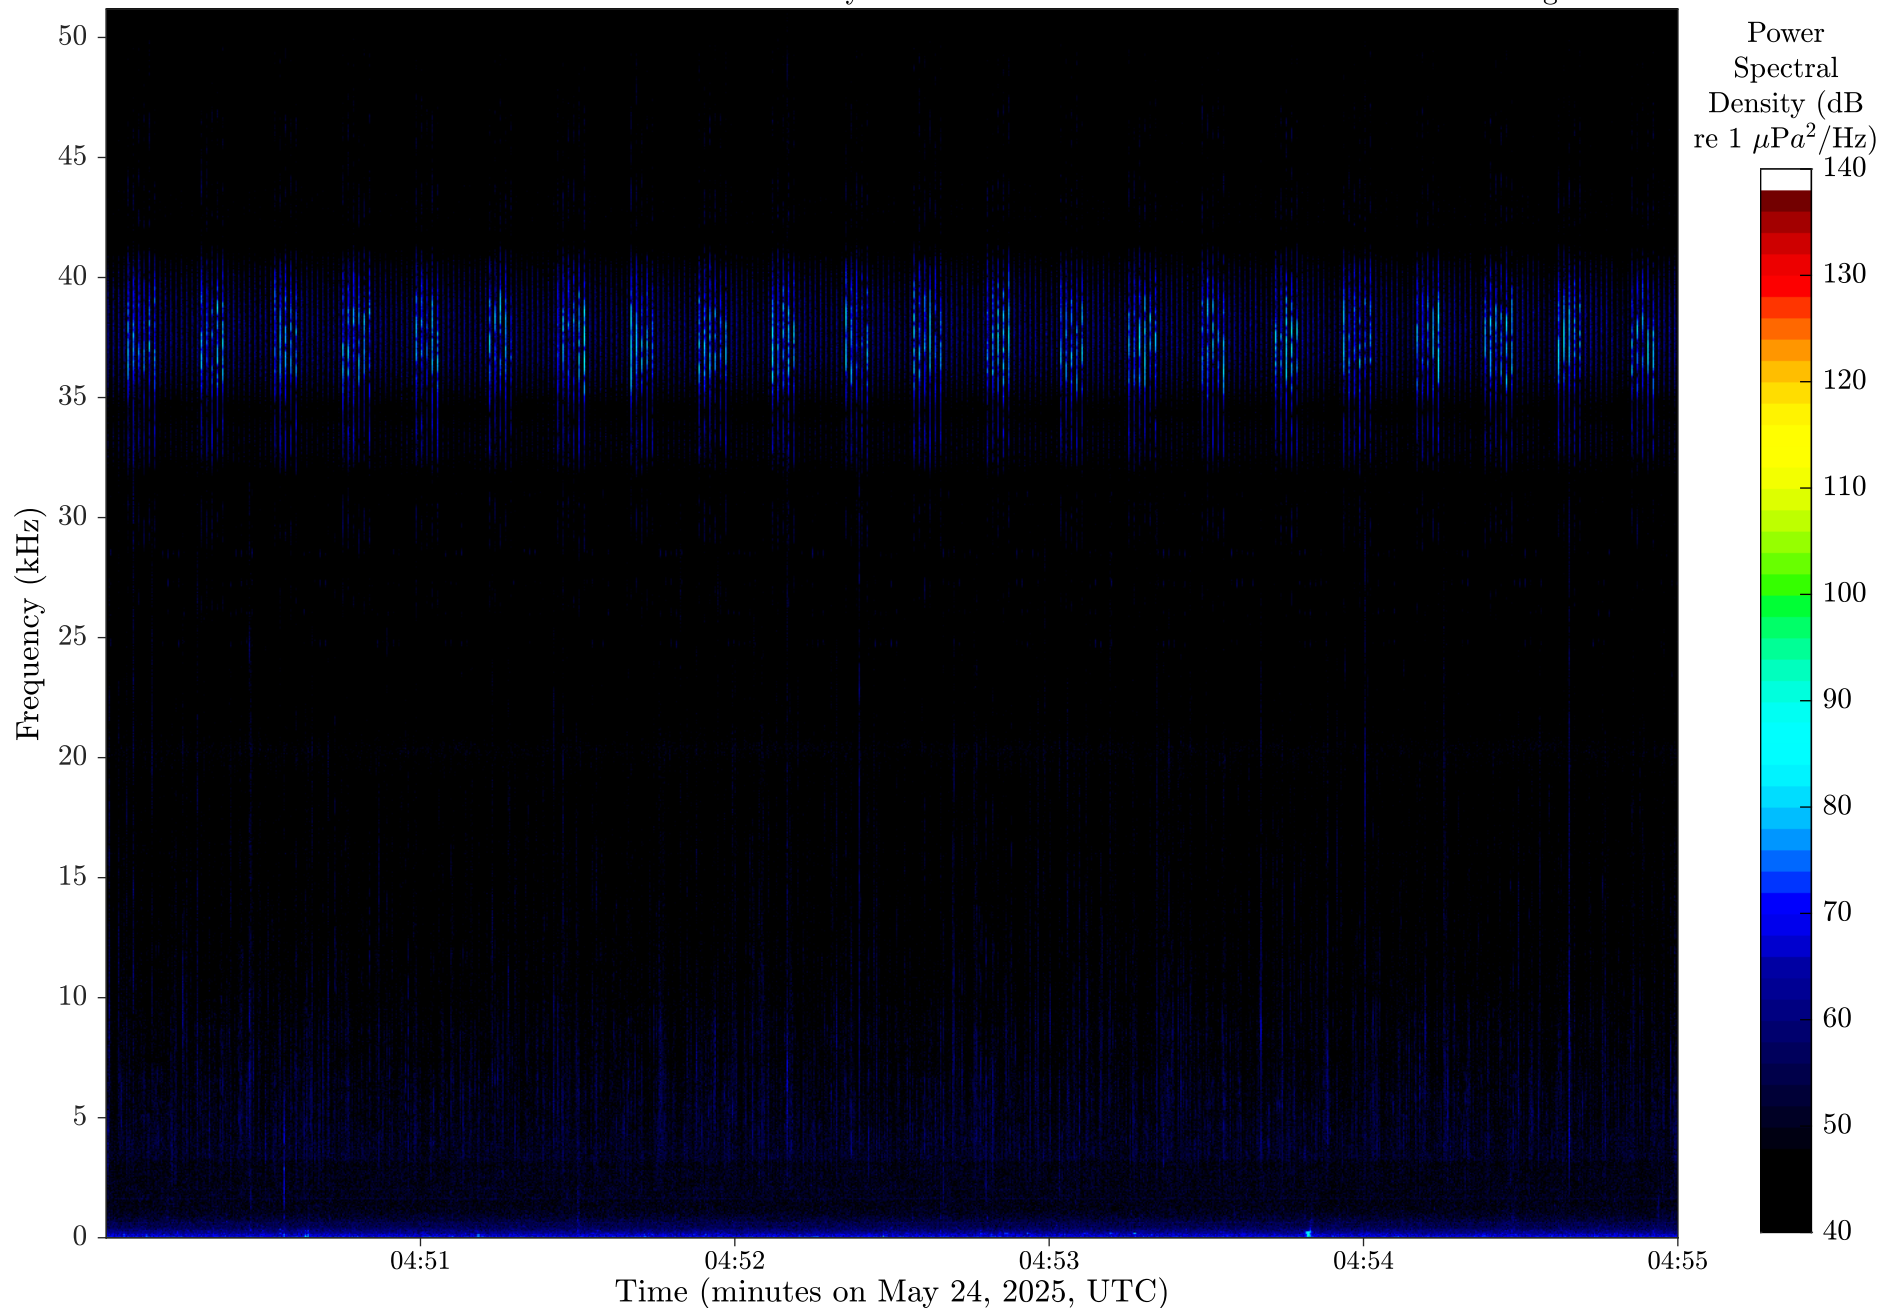


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:55 UTC

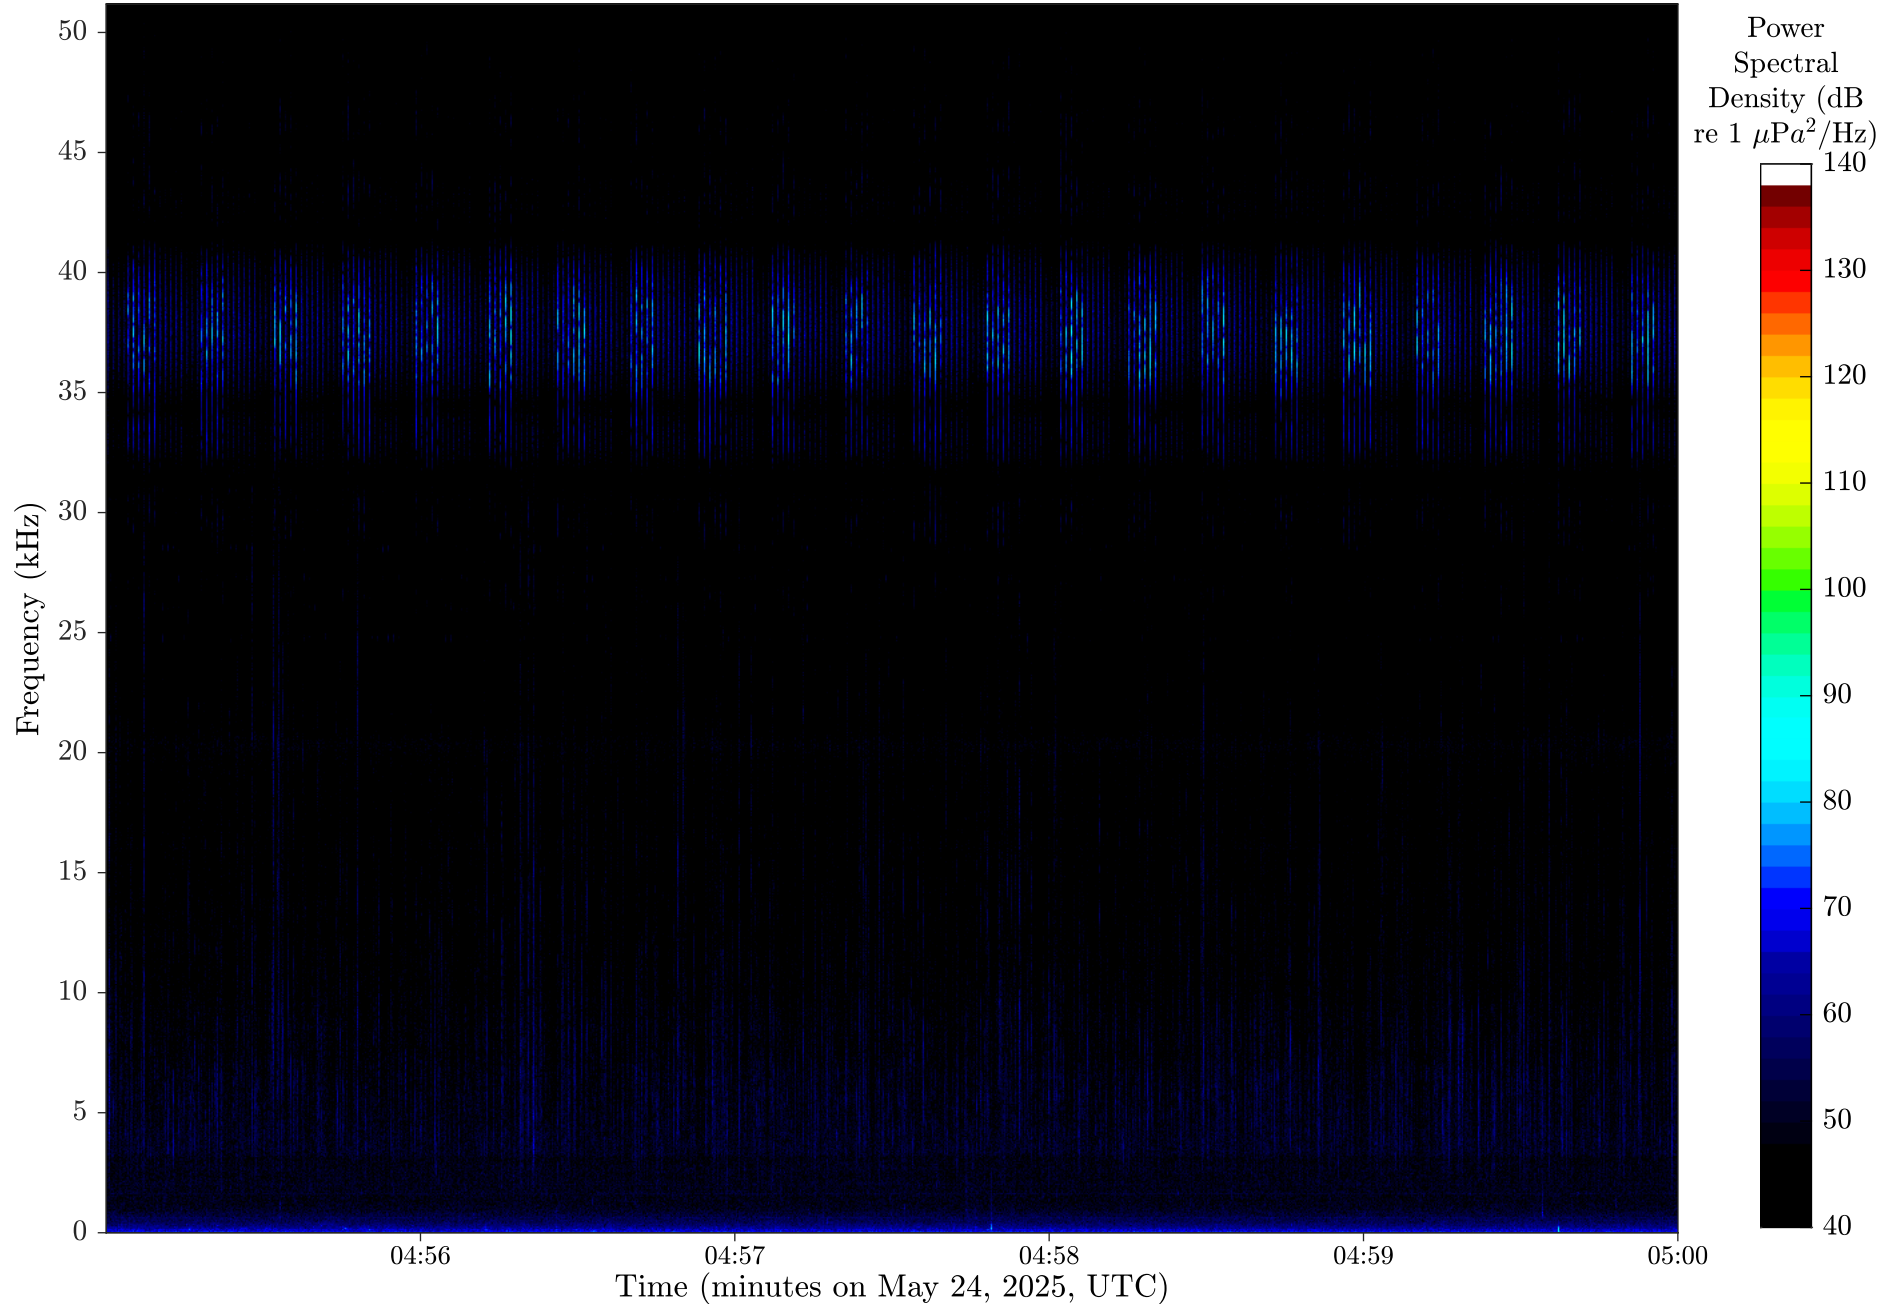


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:23:04 UTC

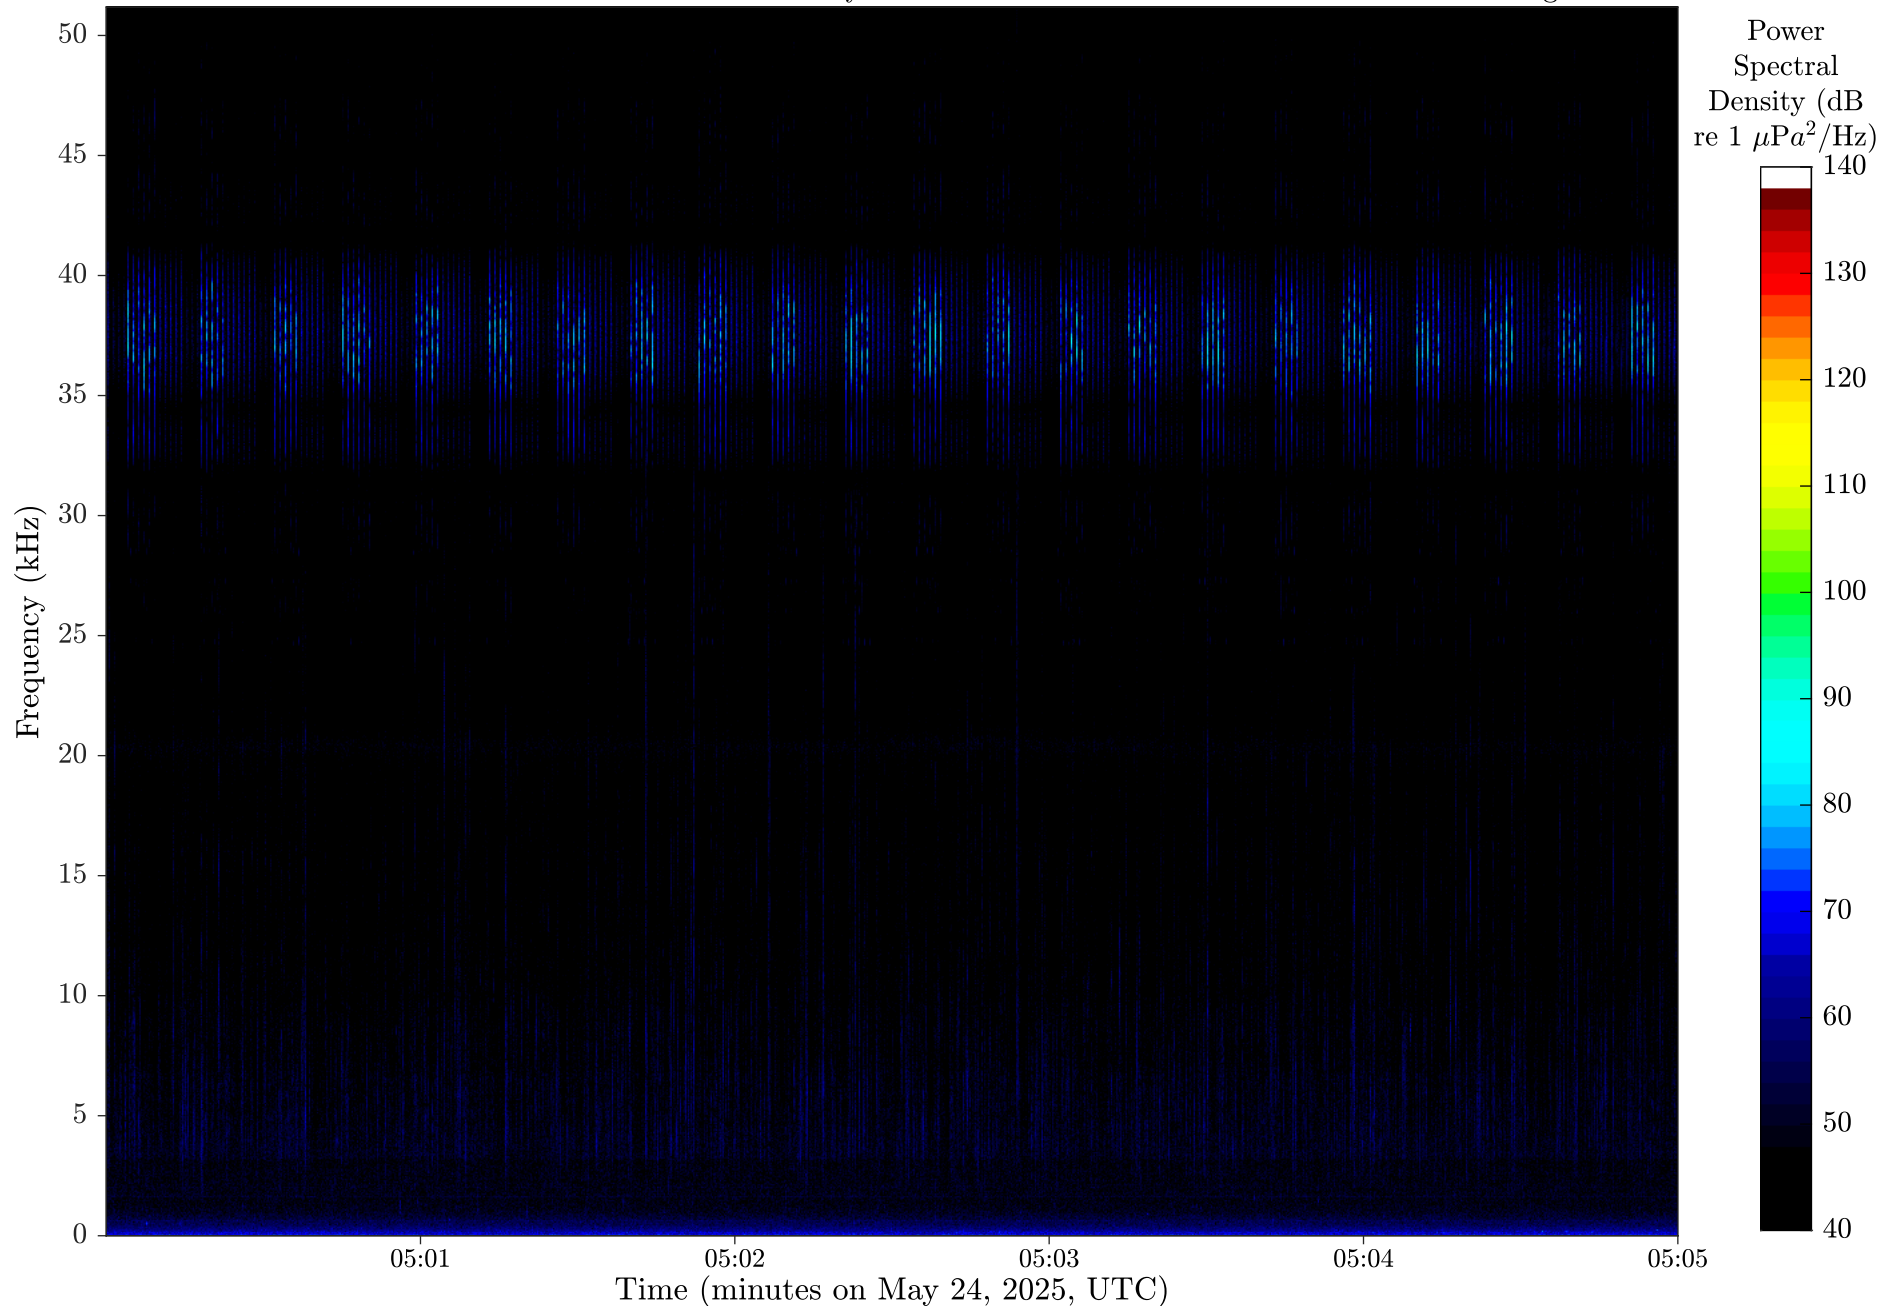

Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:23:13 UTC

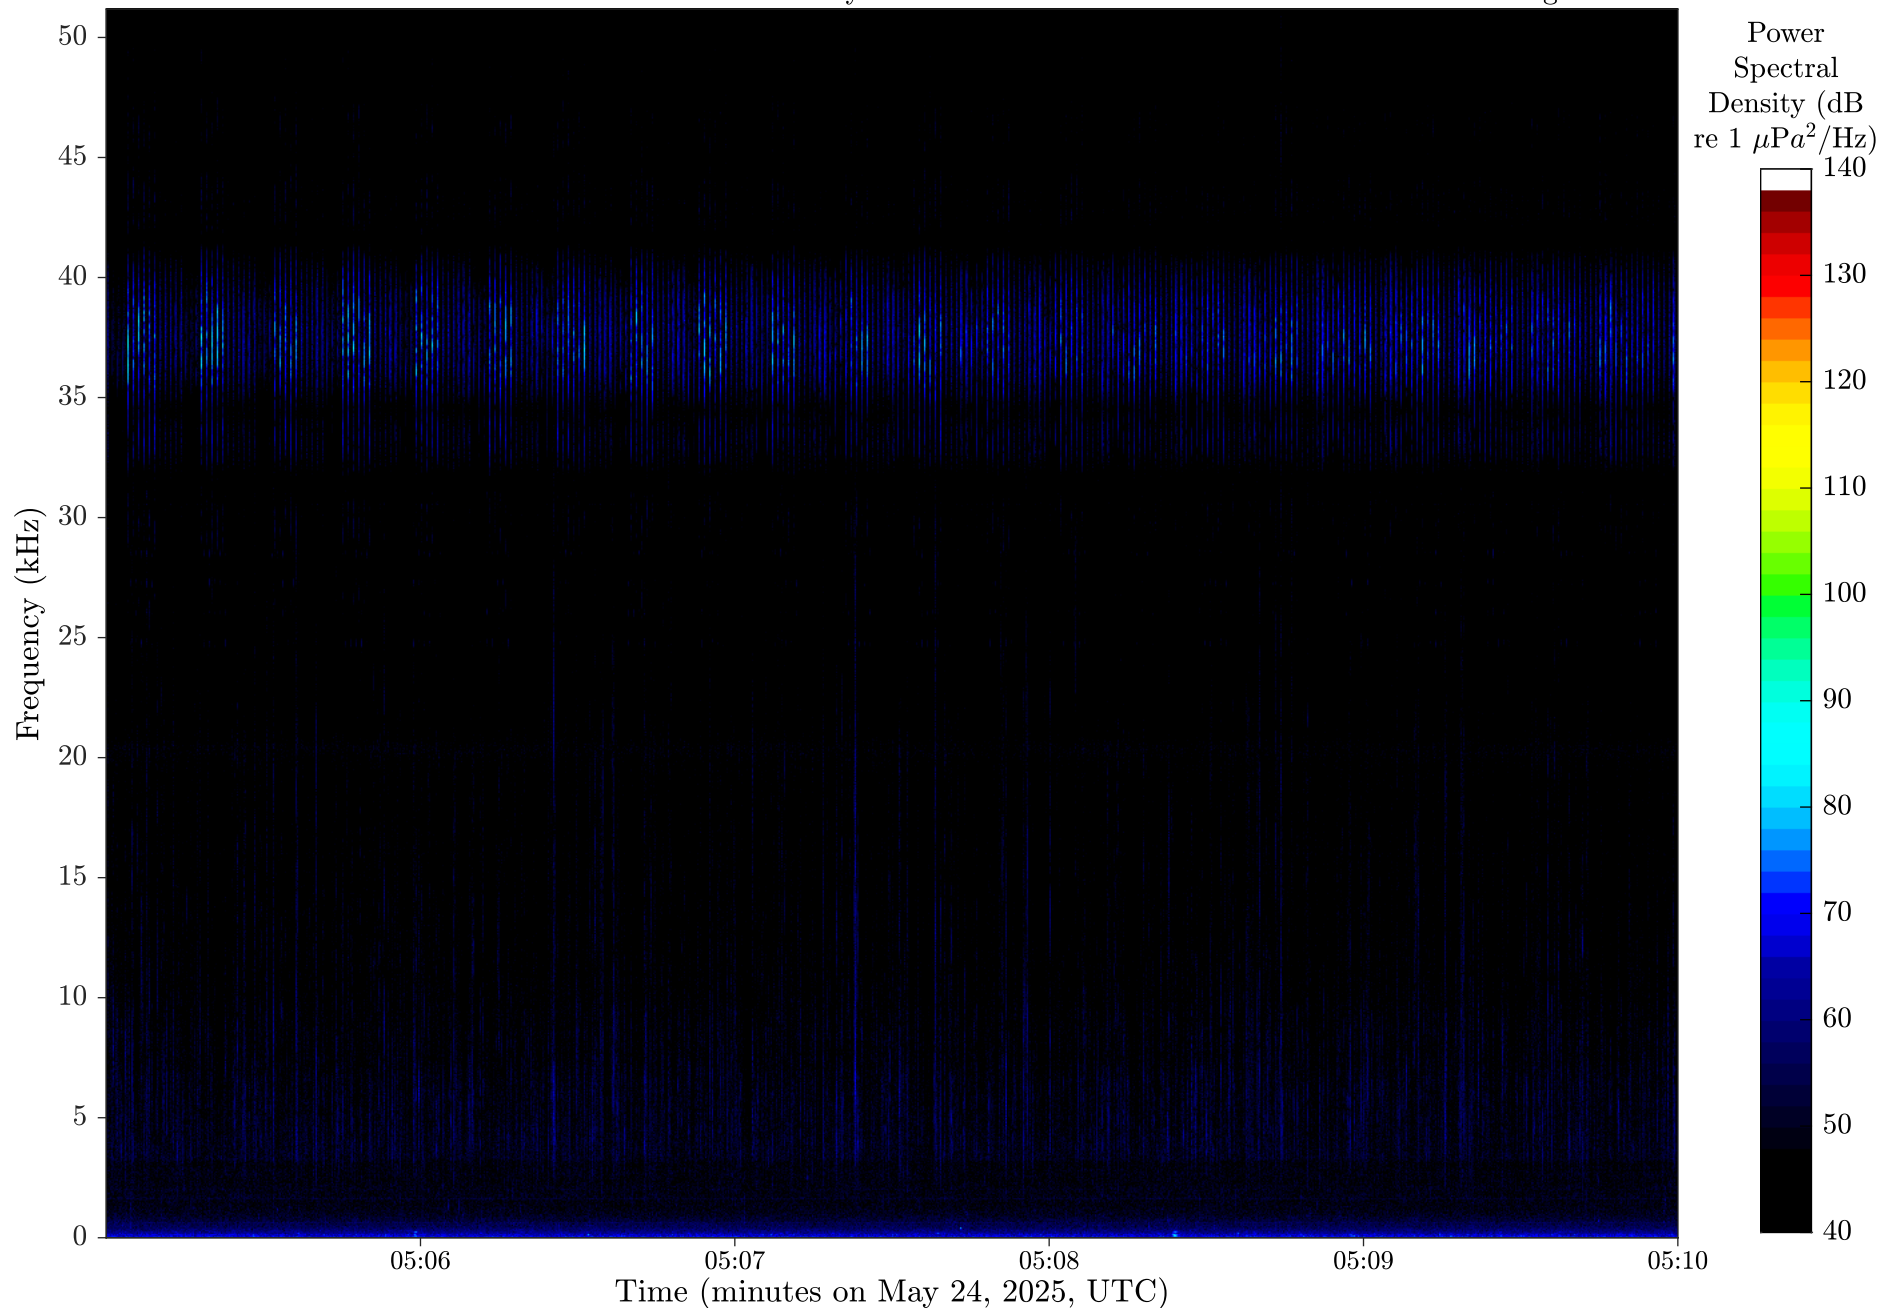


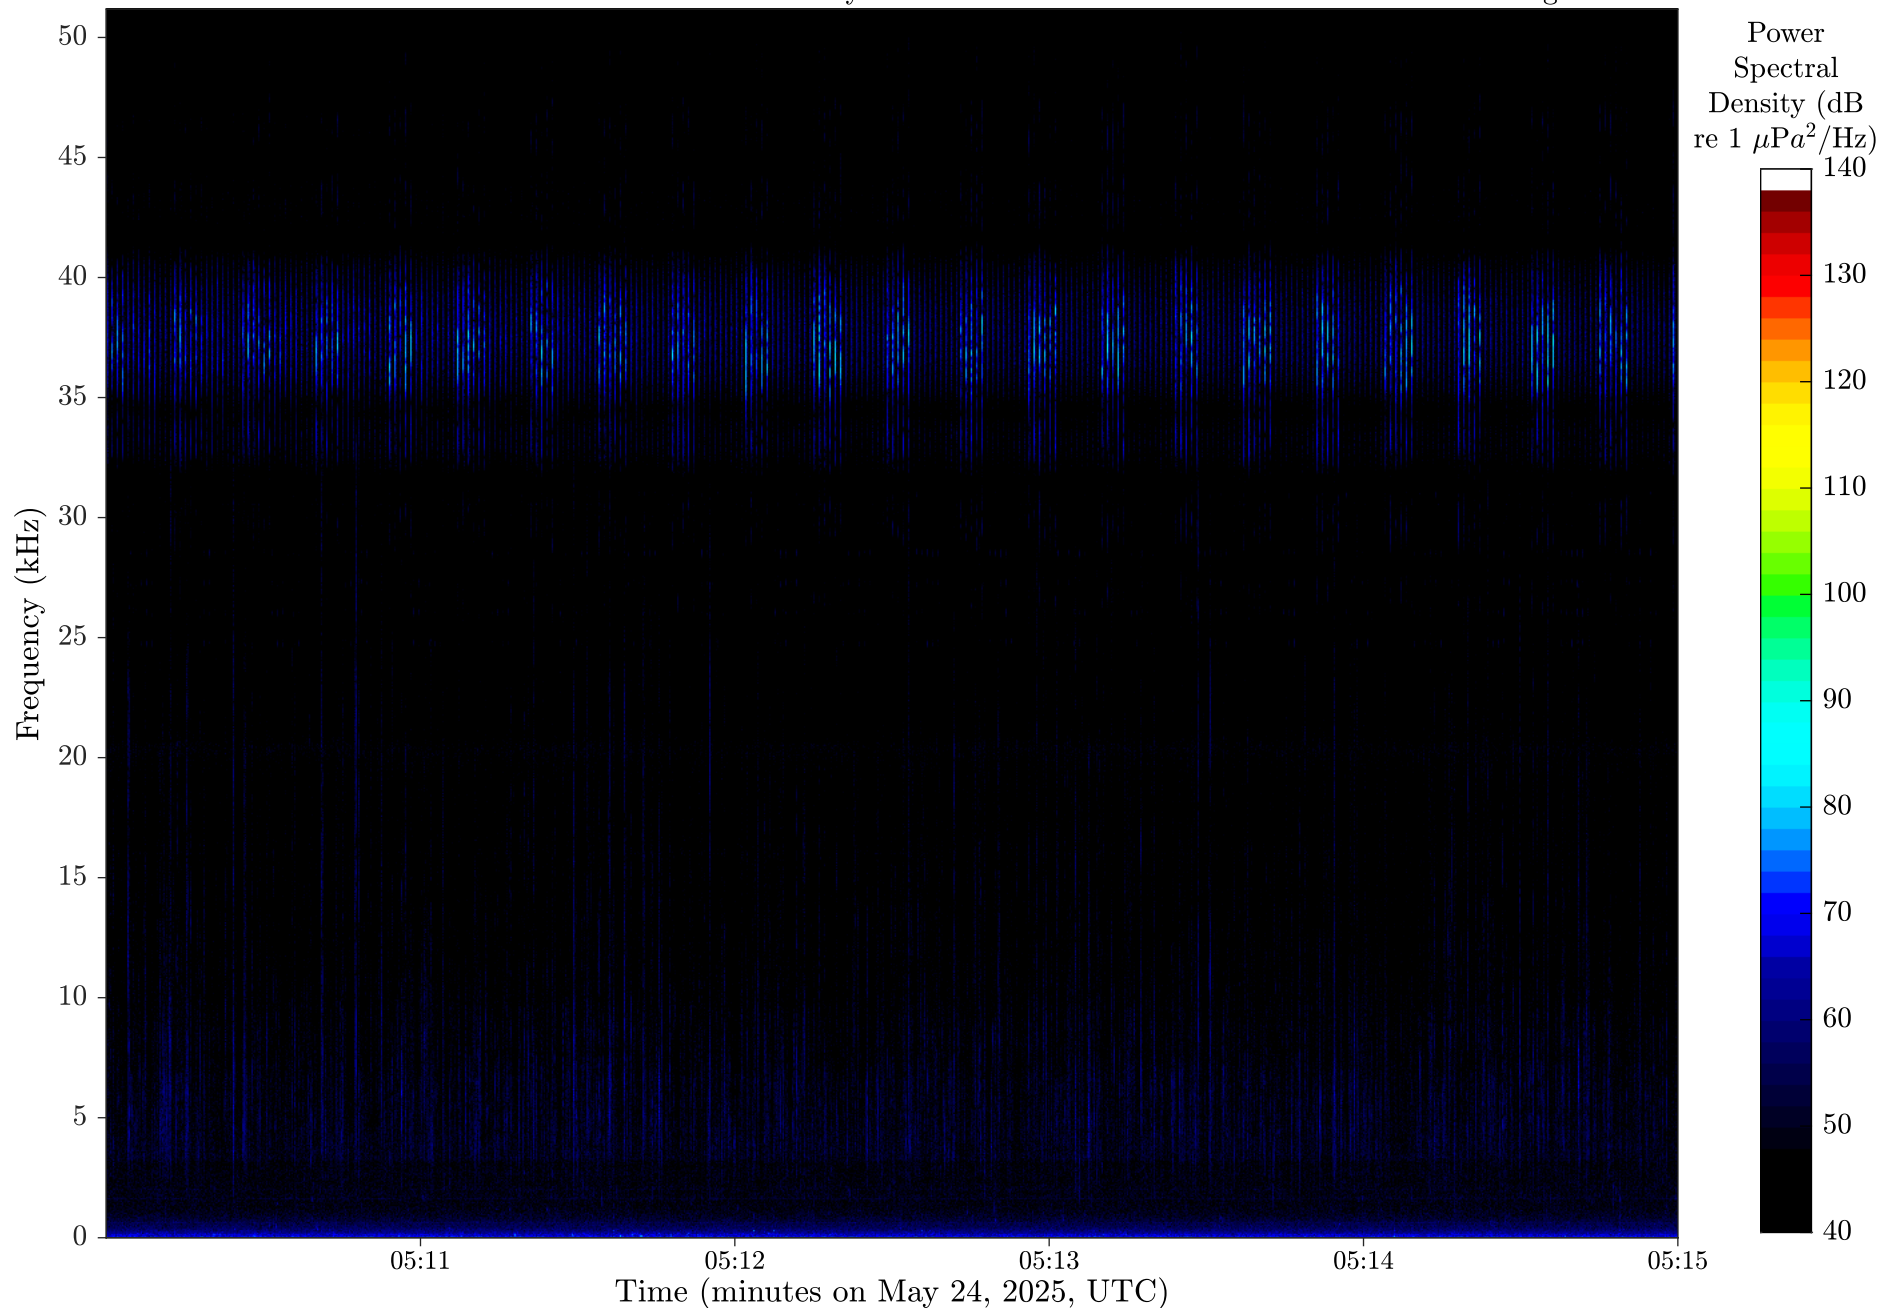

Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:23:30 UTC

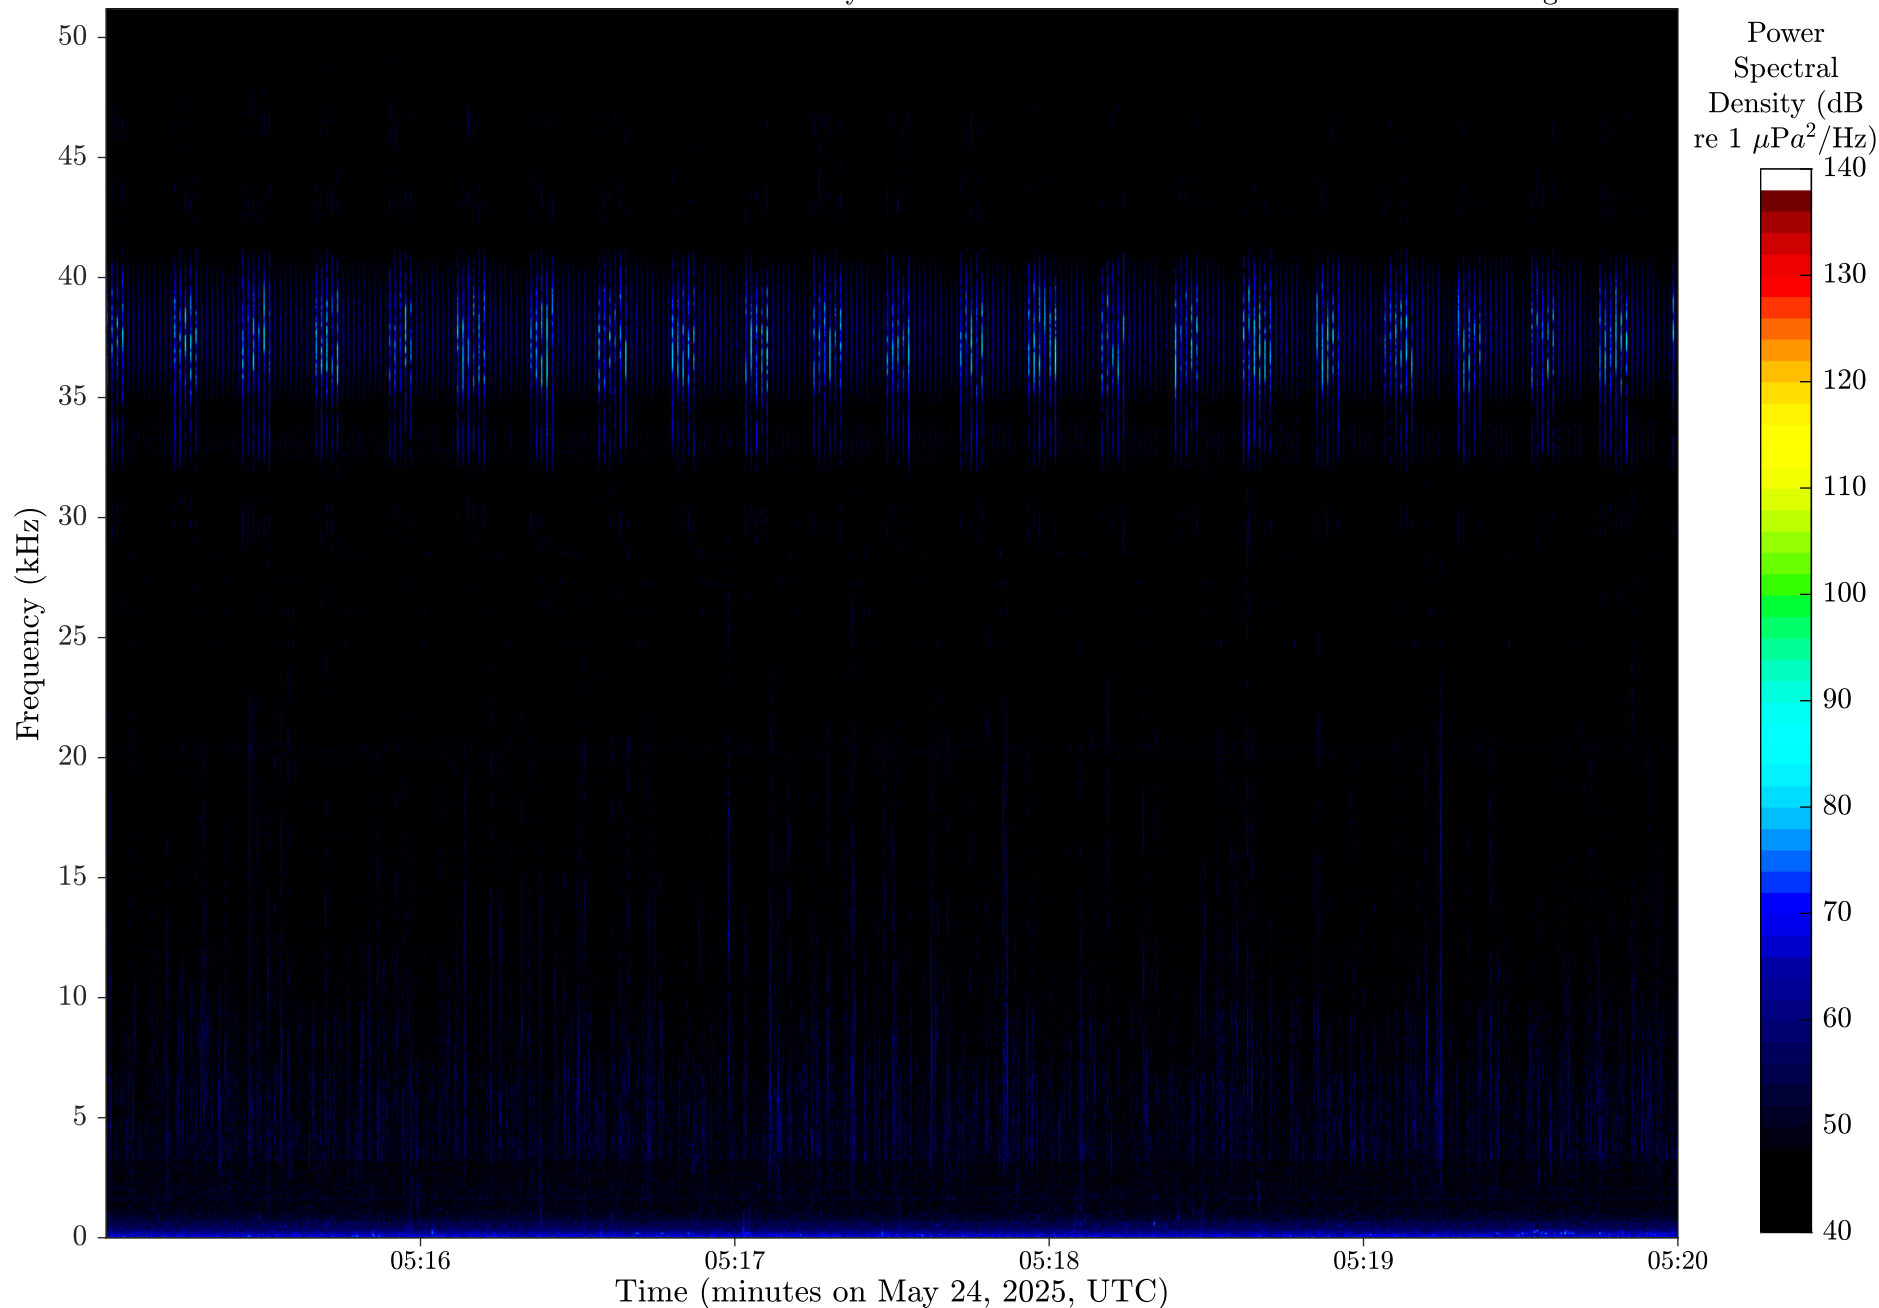

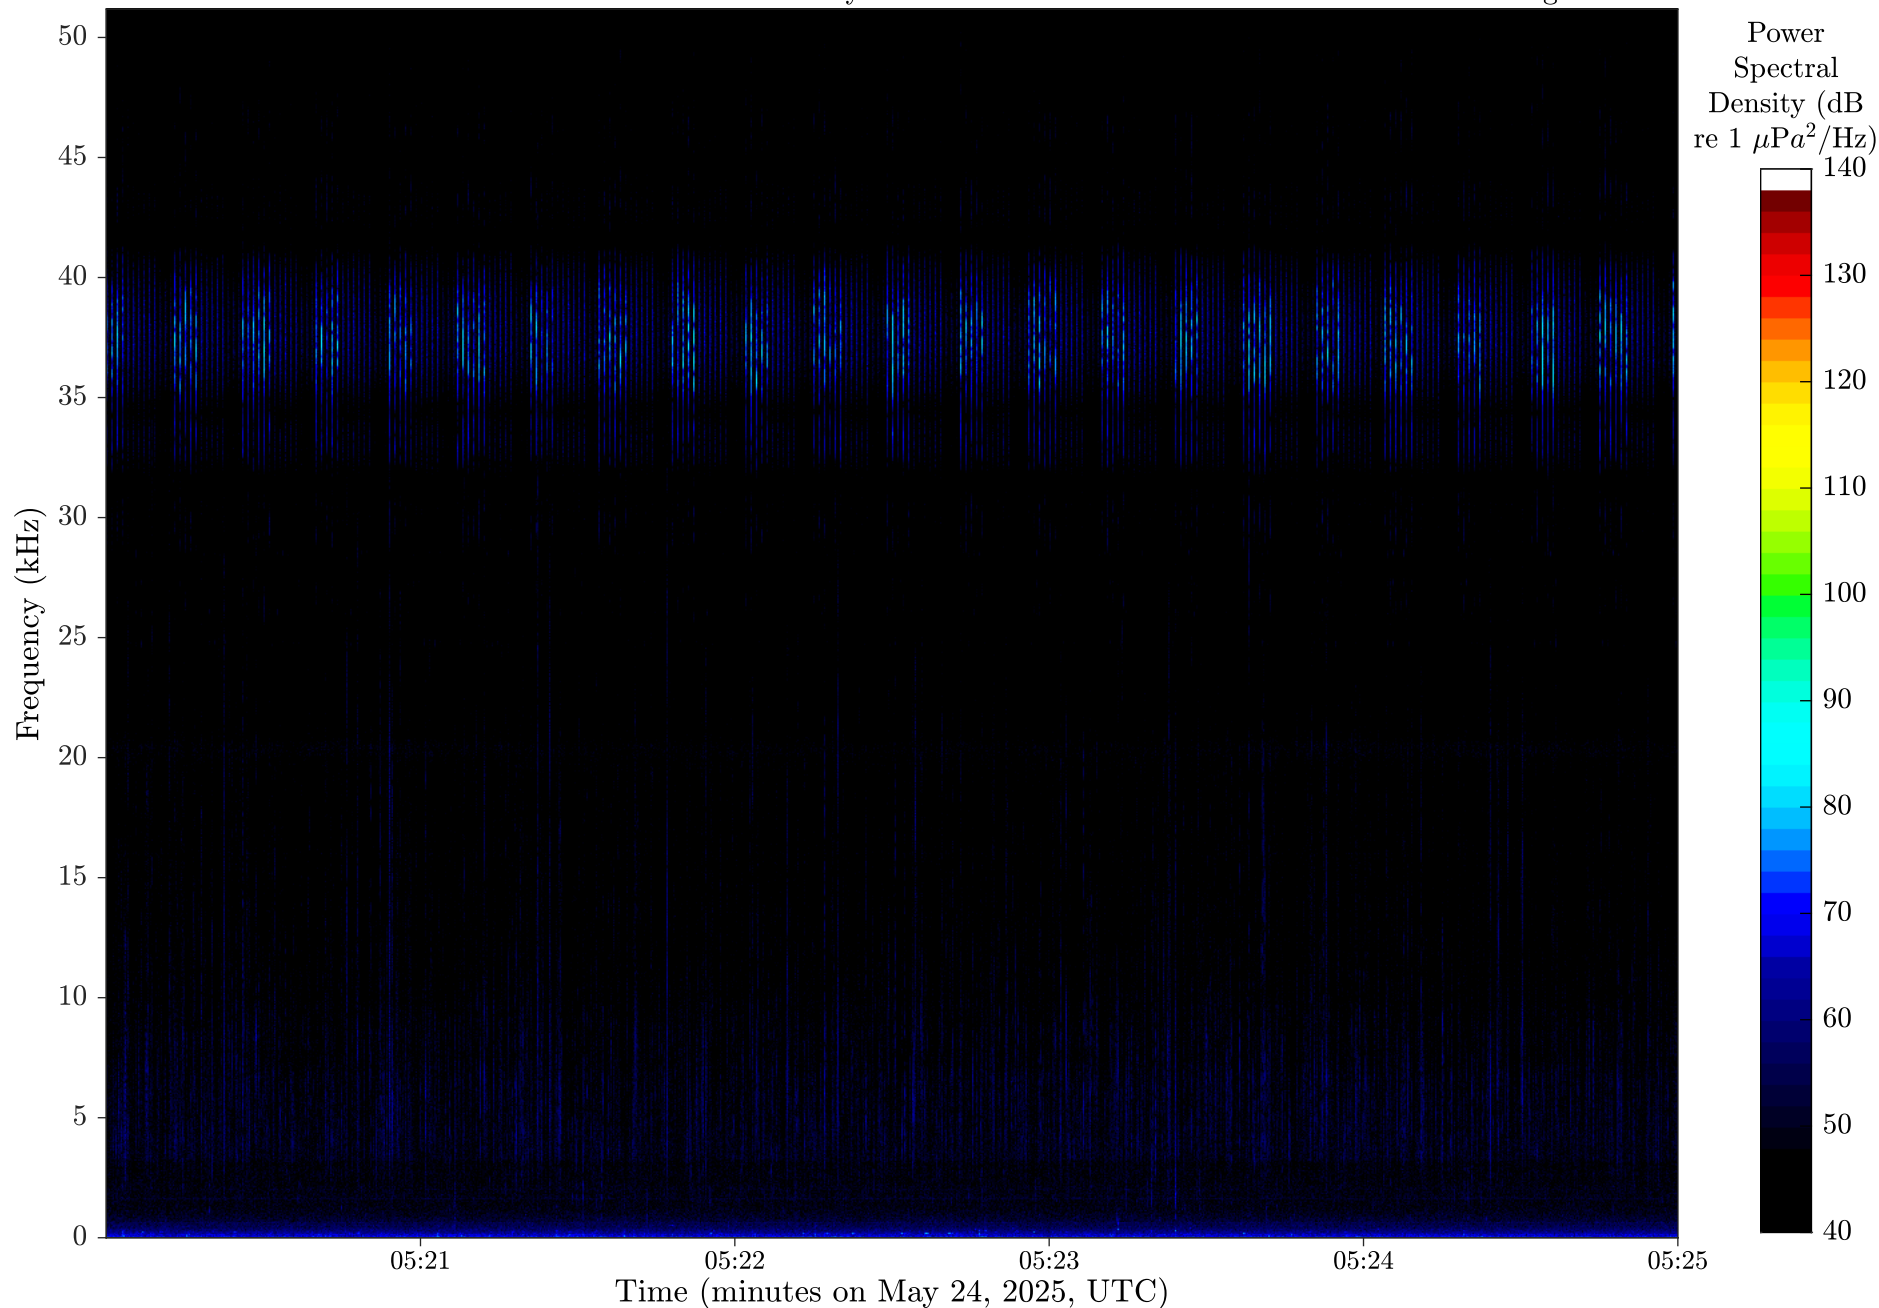


Comments: 36.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:46 UTC

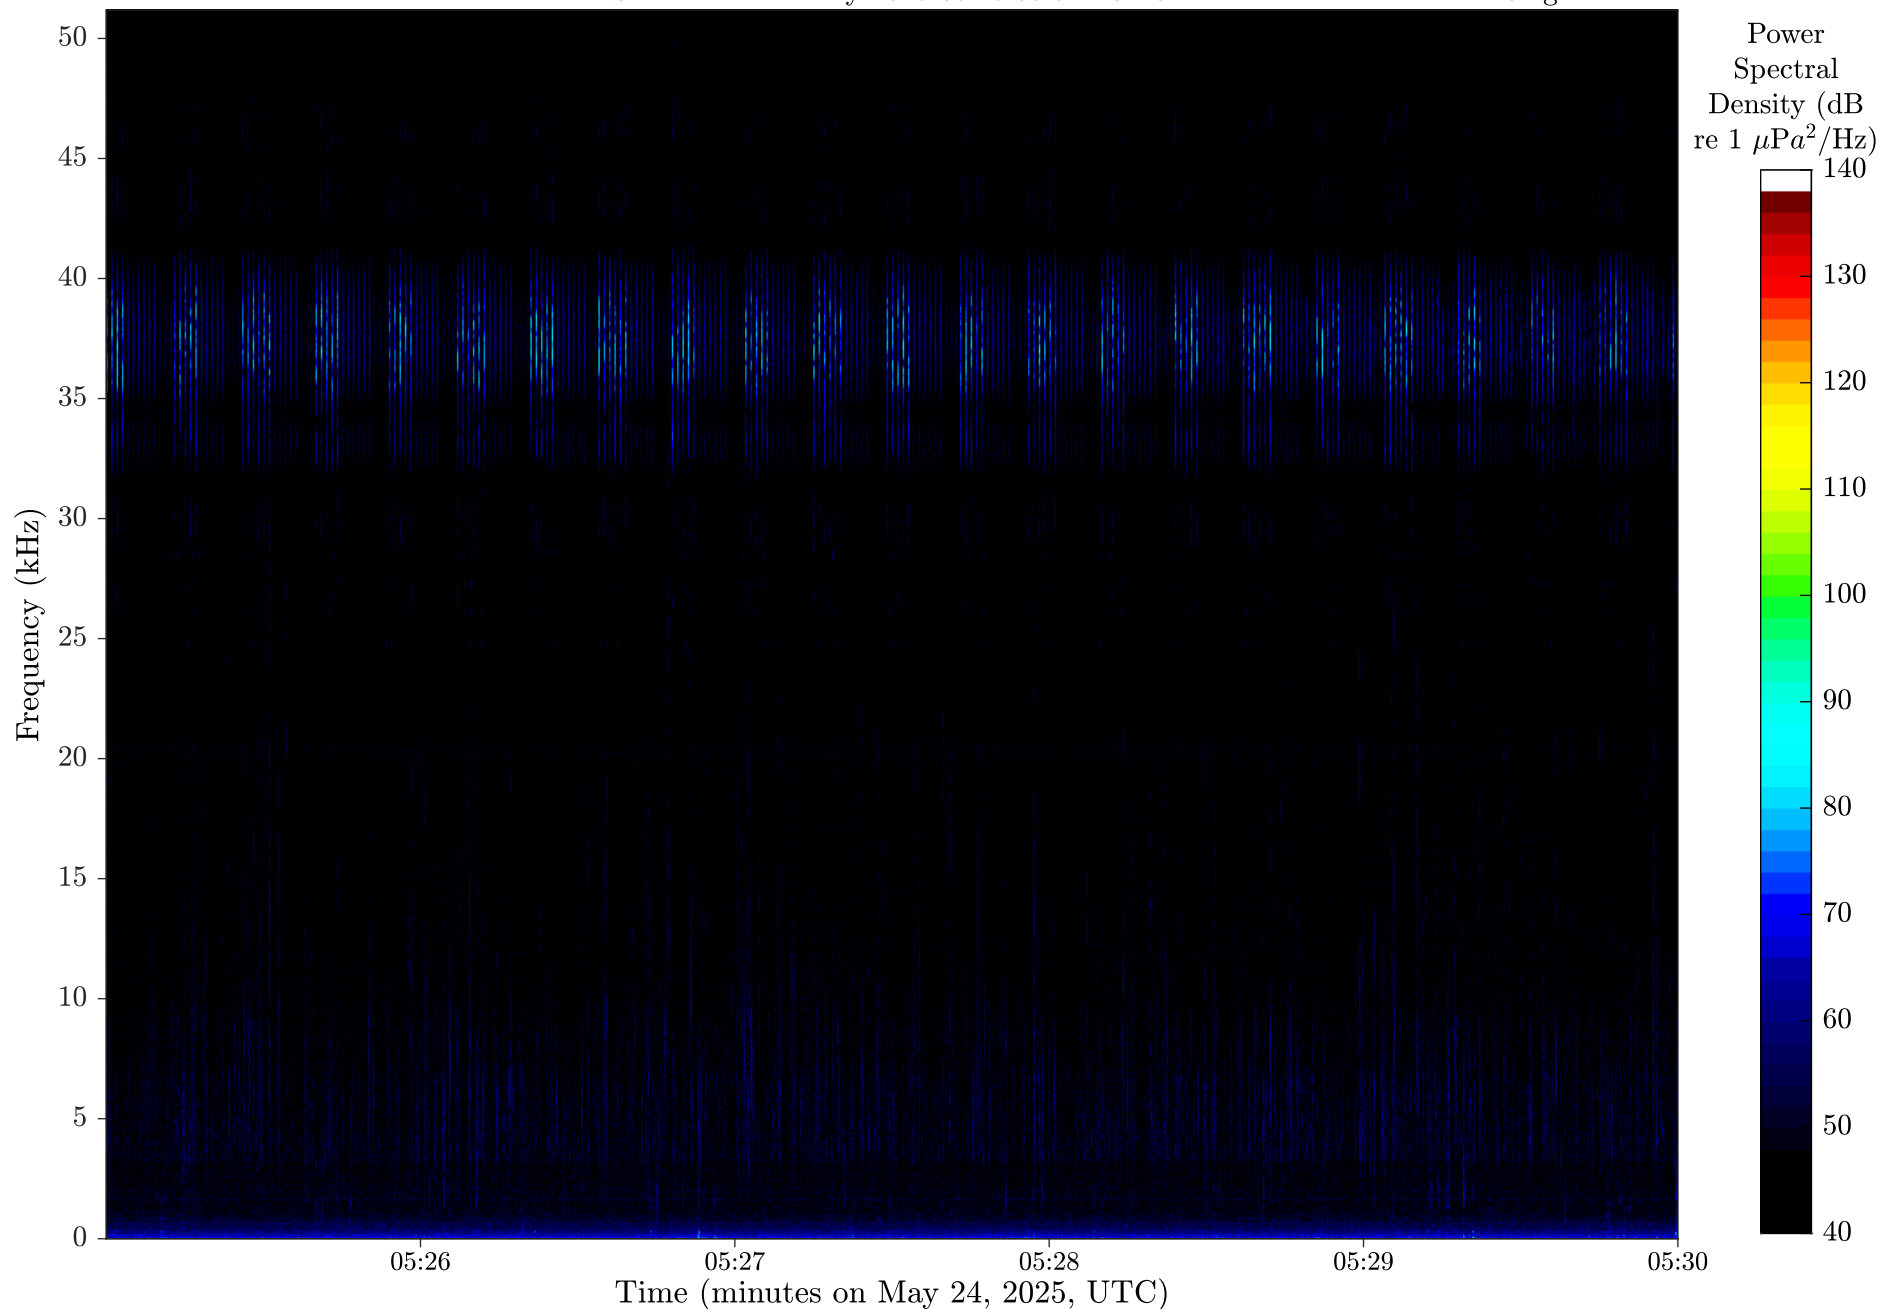


Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:55 UTC

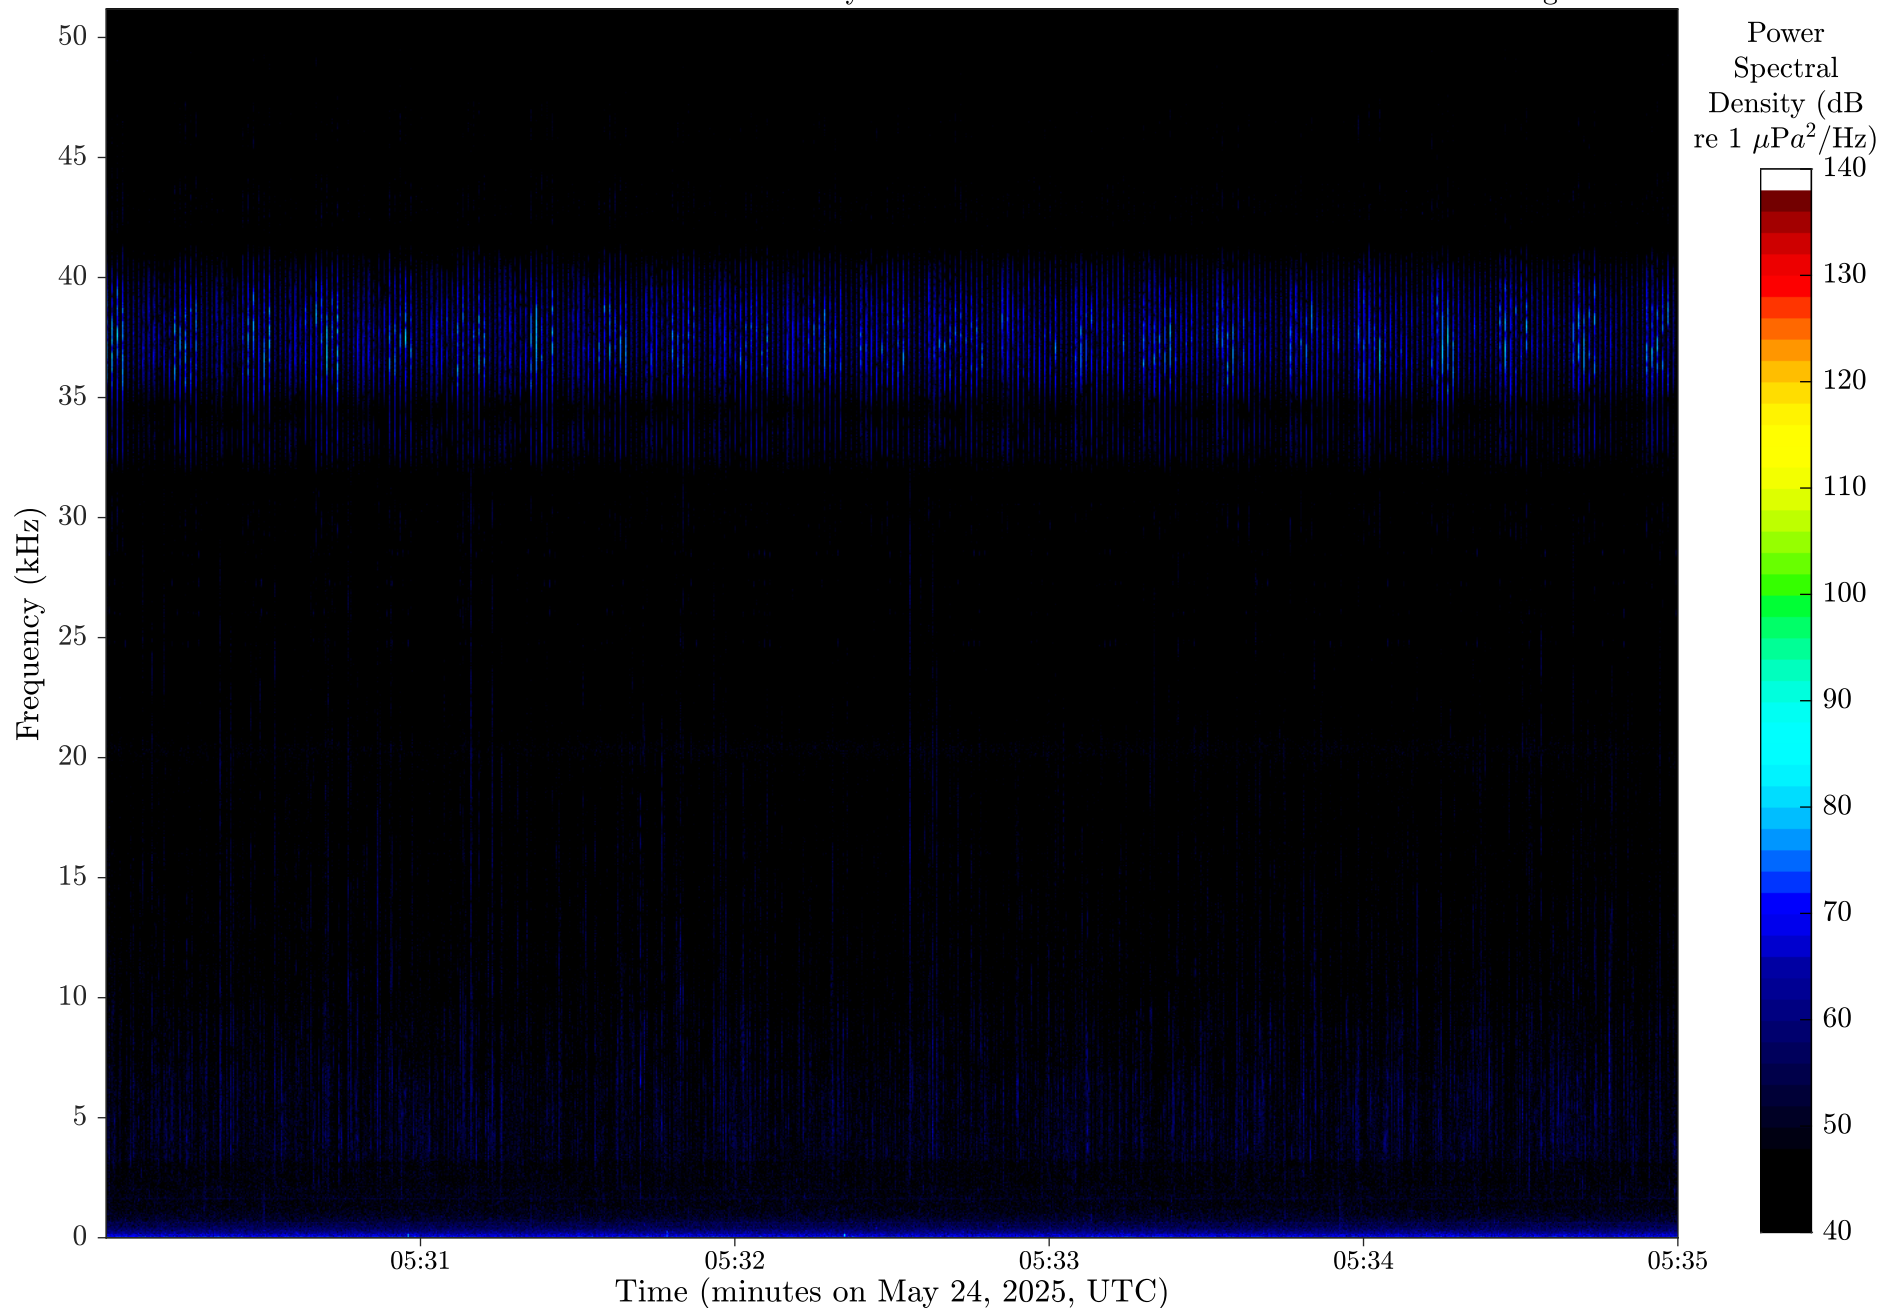


Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:24:03 UTC

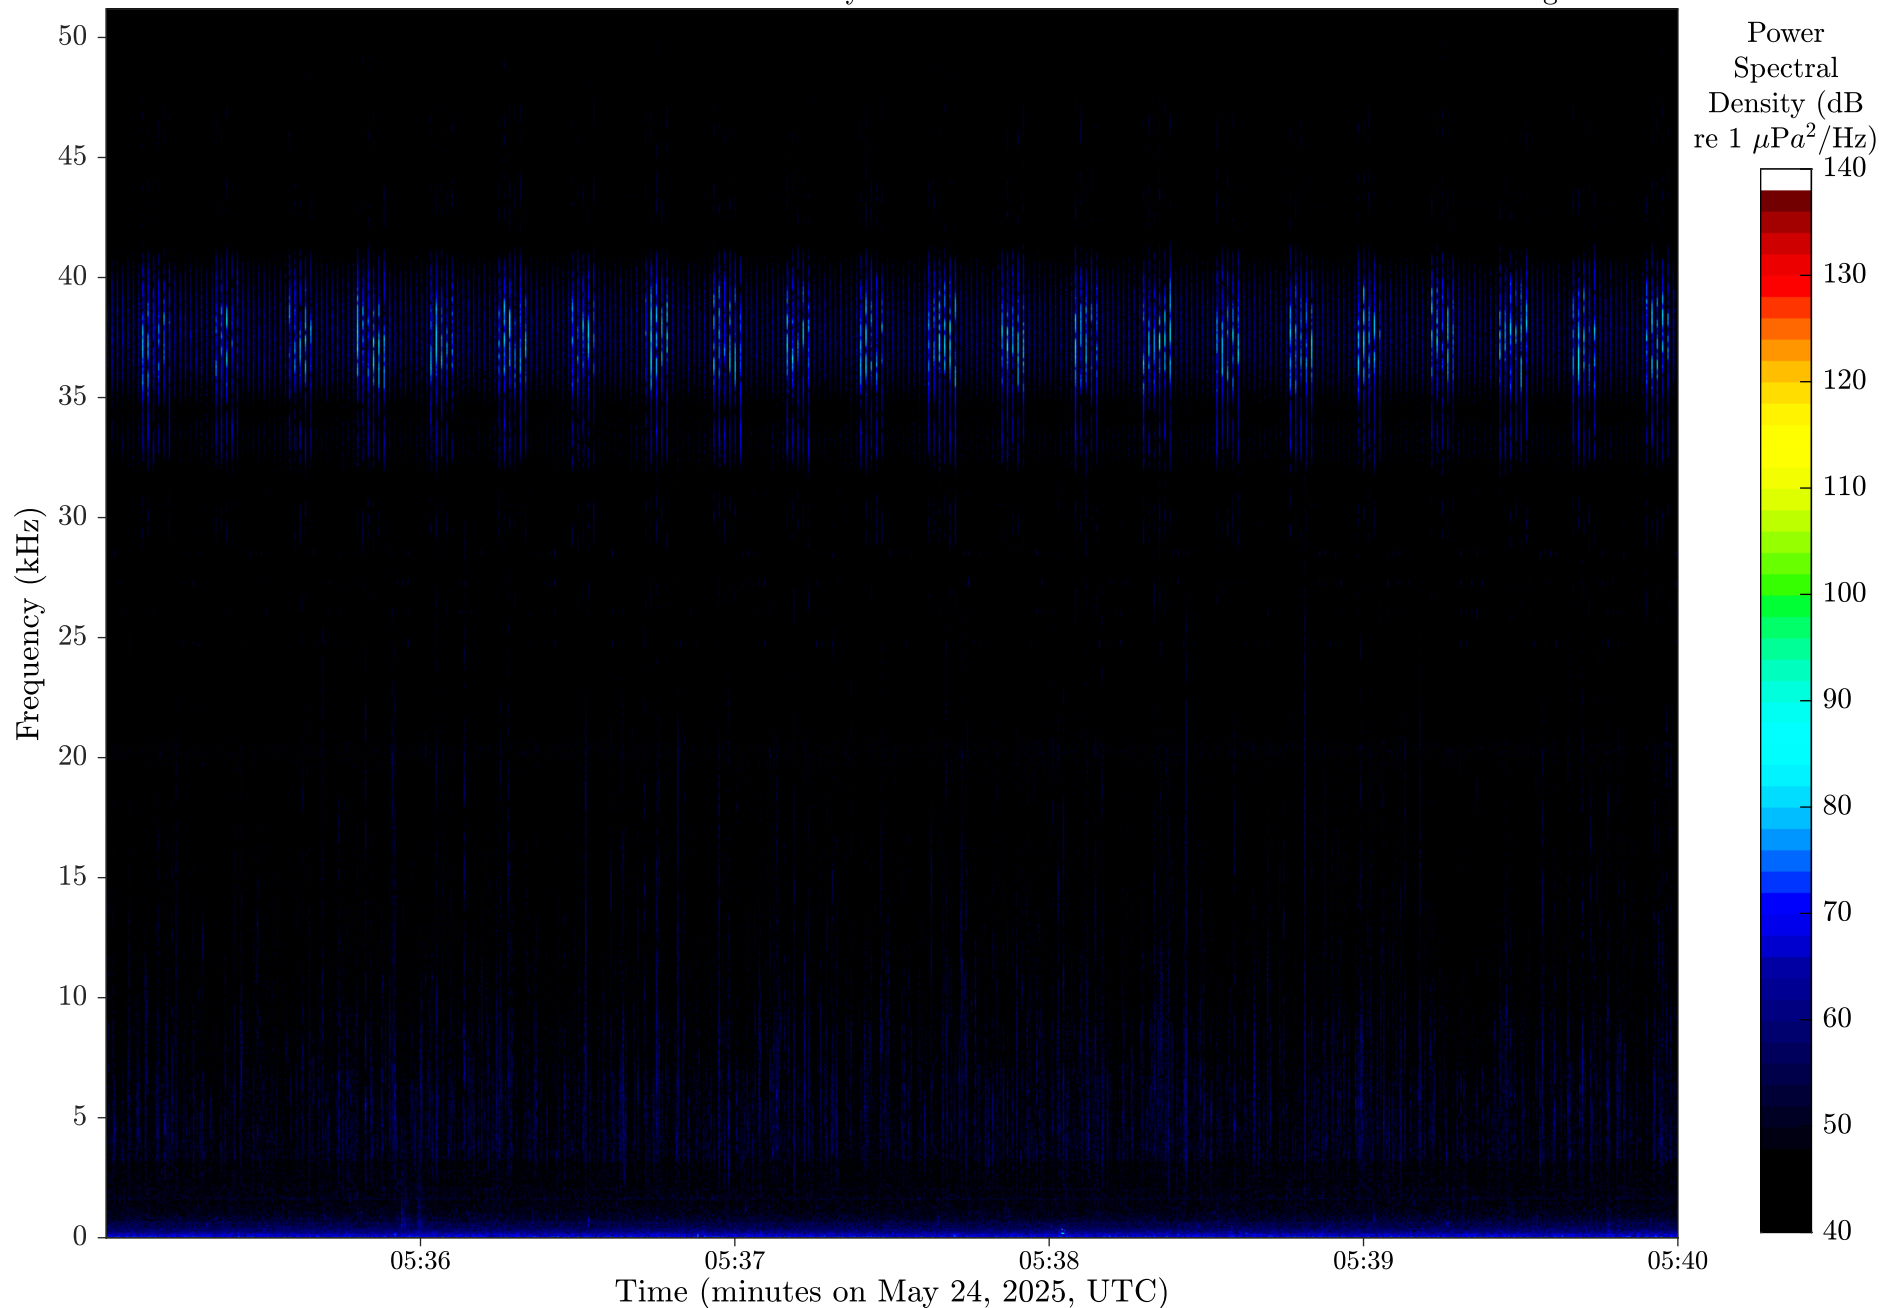

Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:24:12 UTC

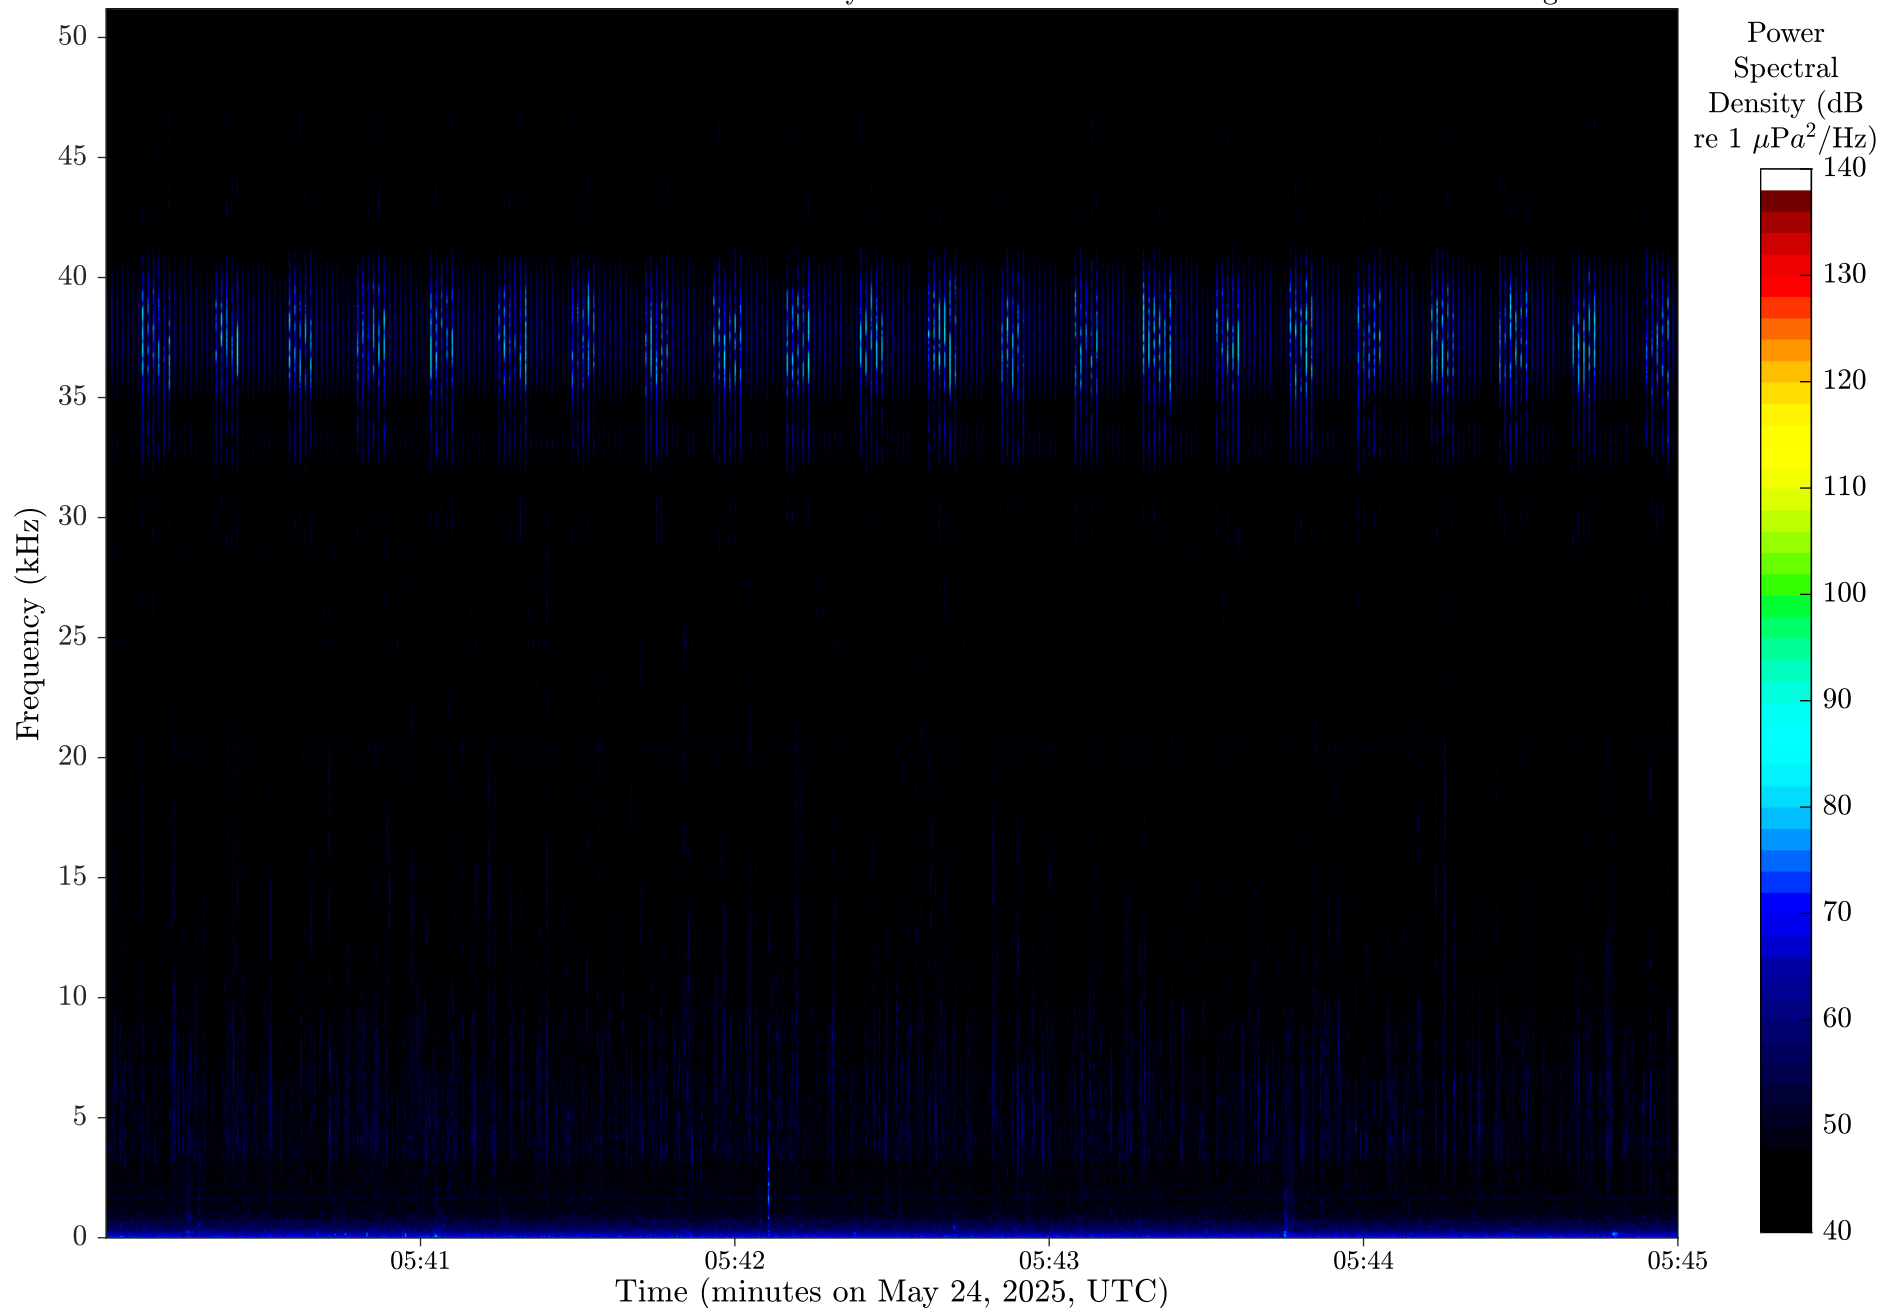

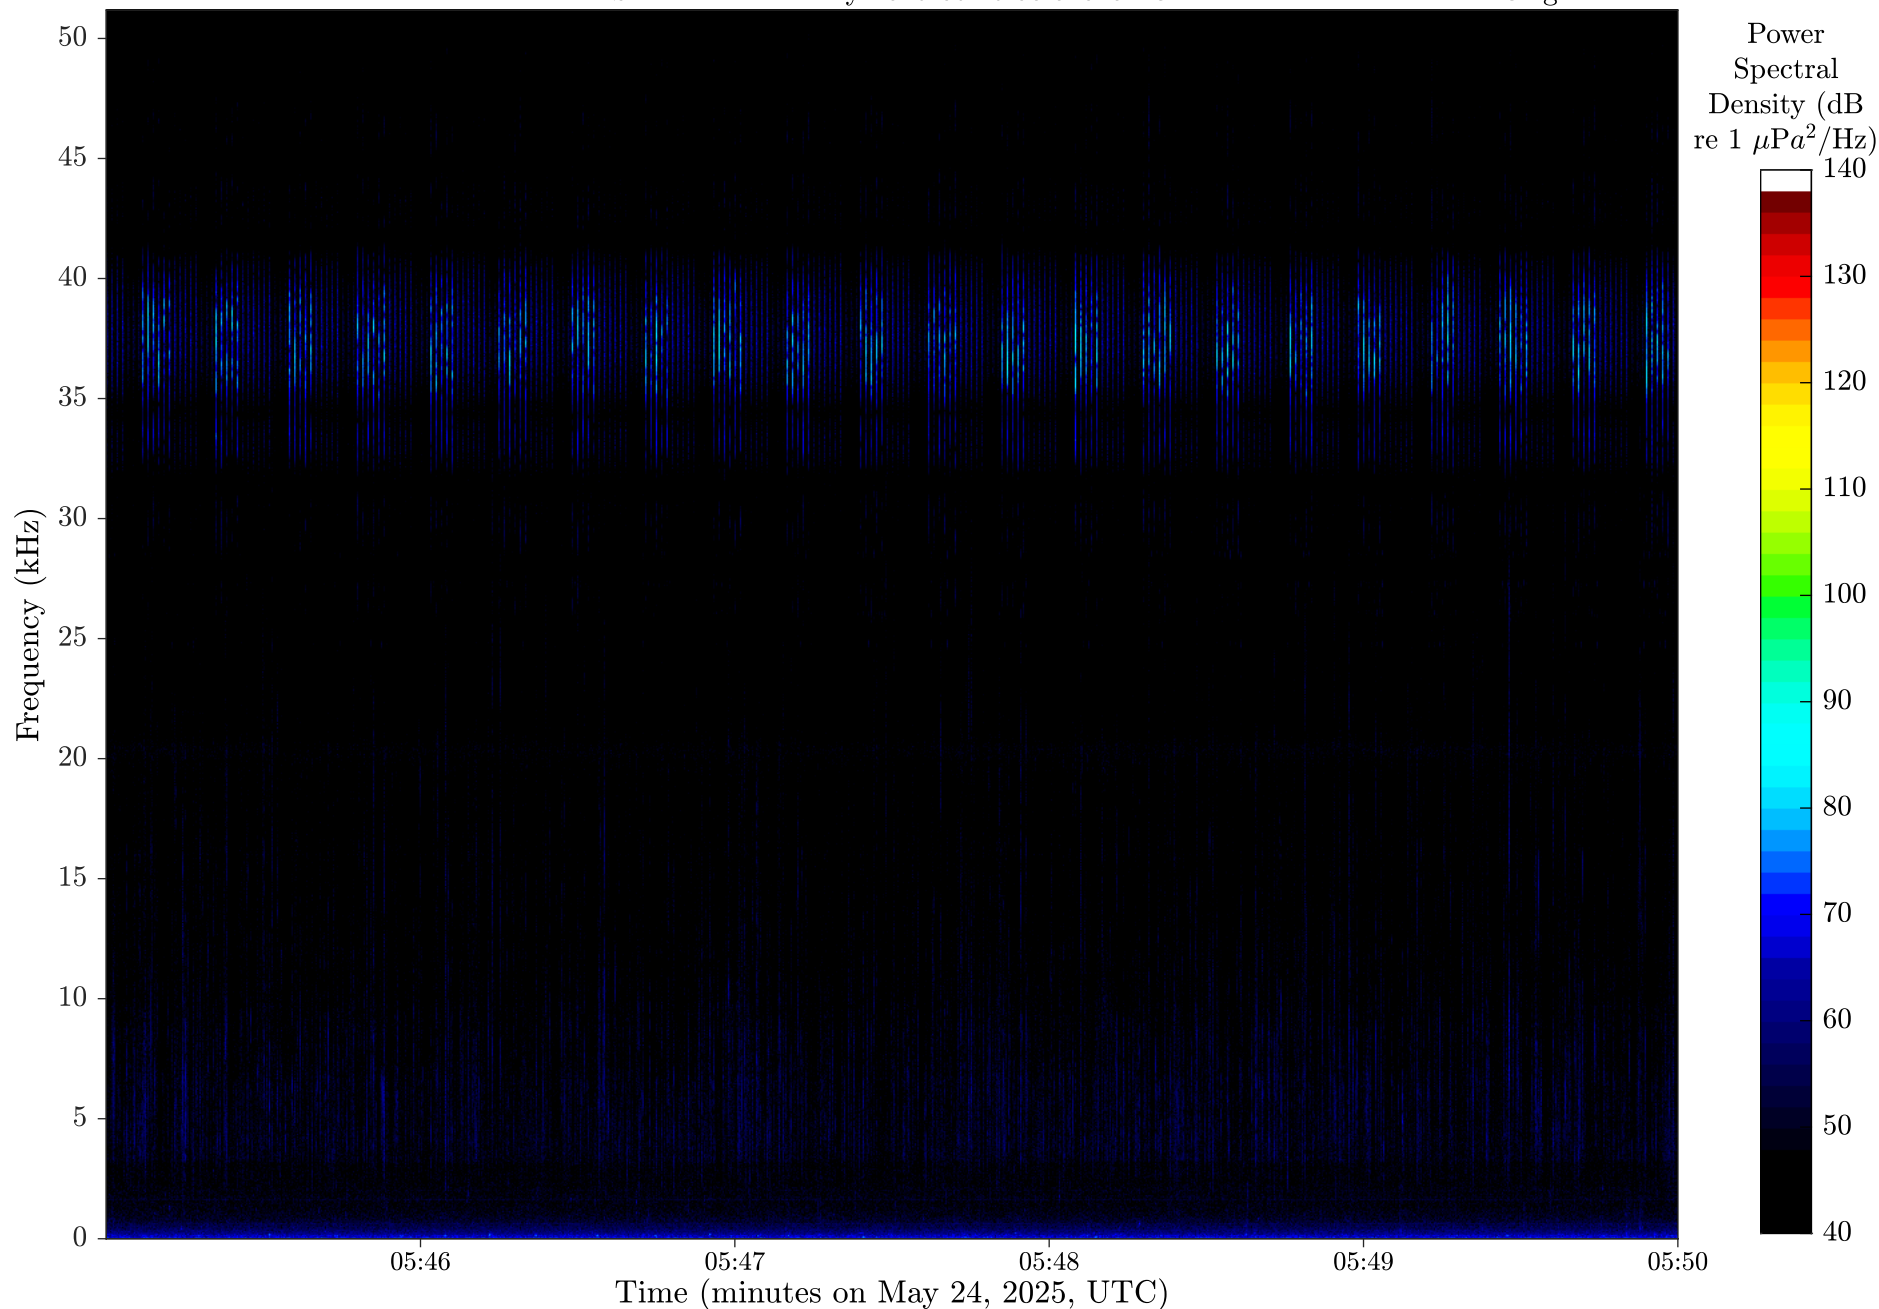


Comments: 36.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:24:29 UTC

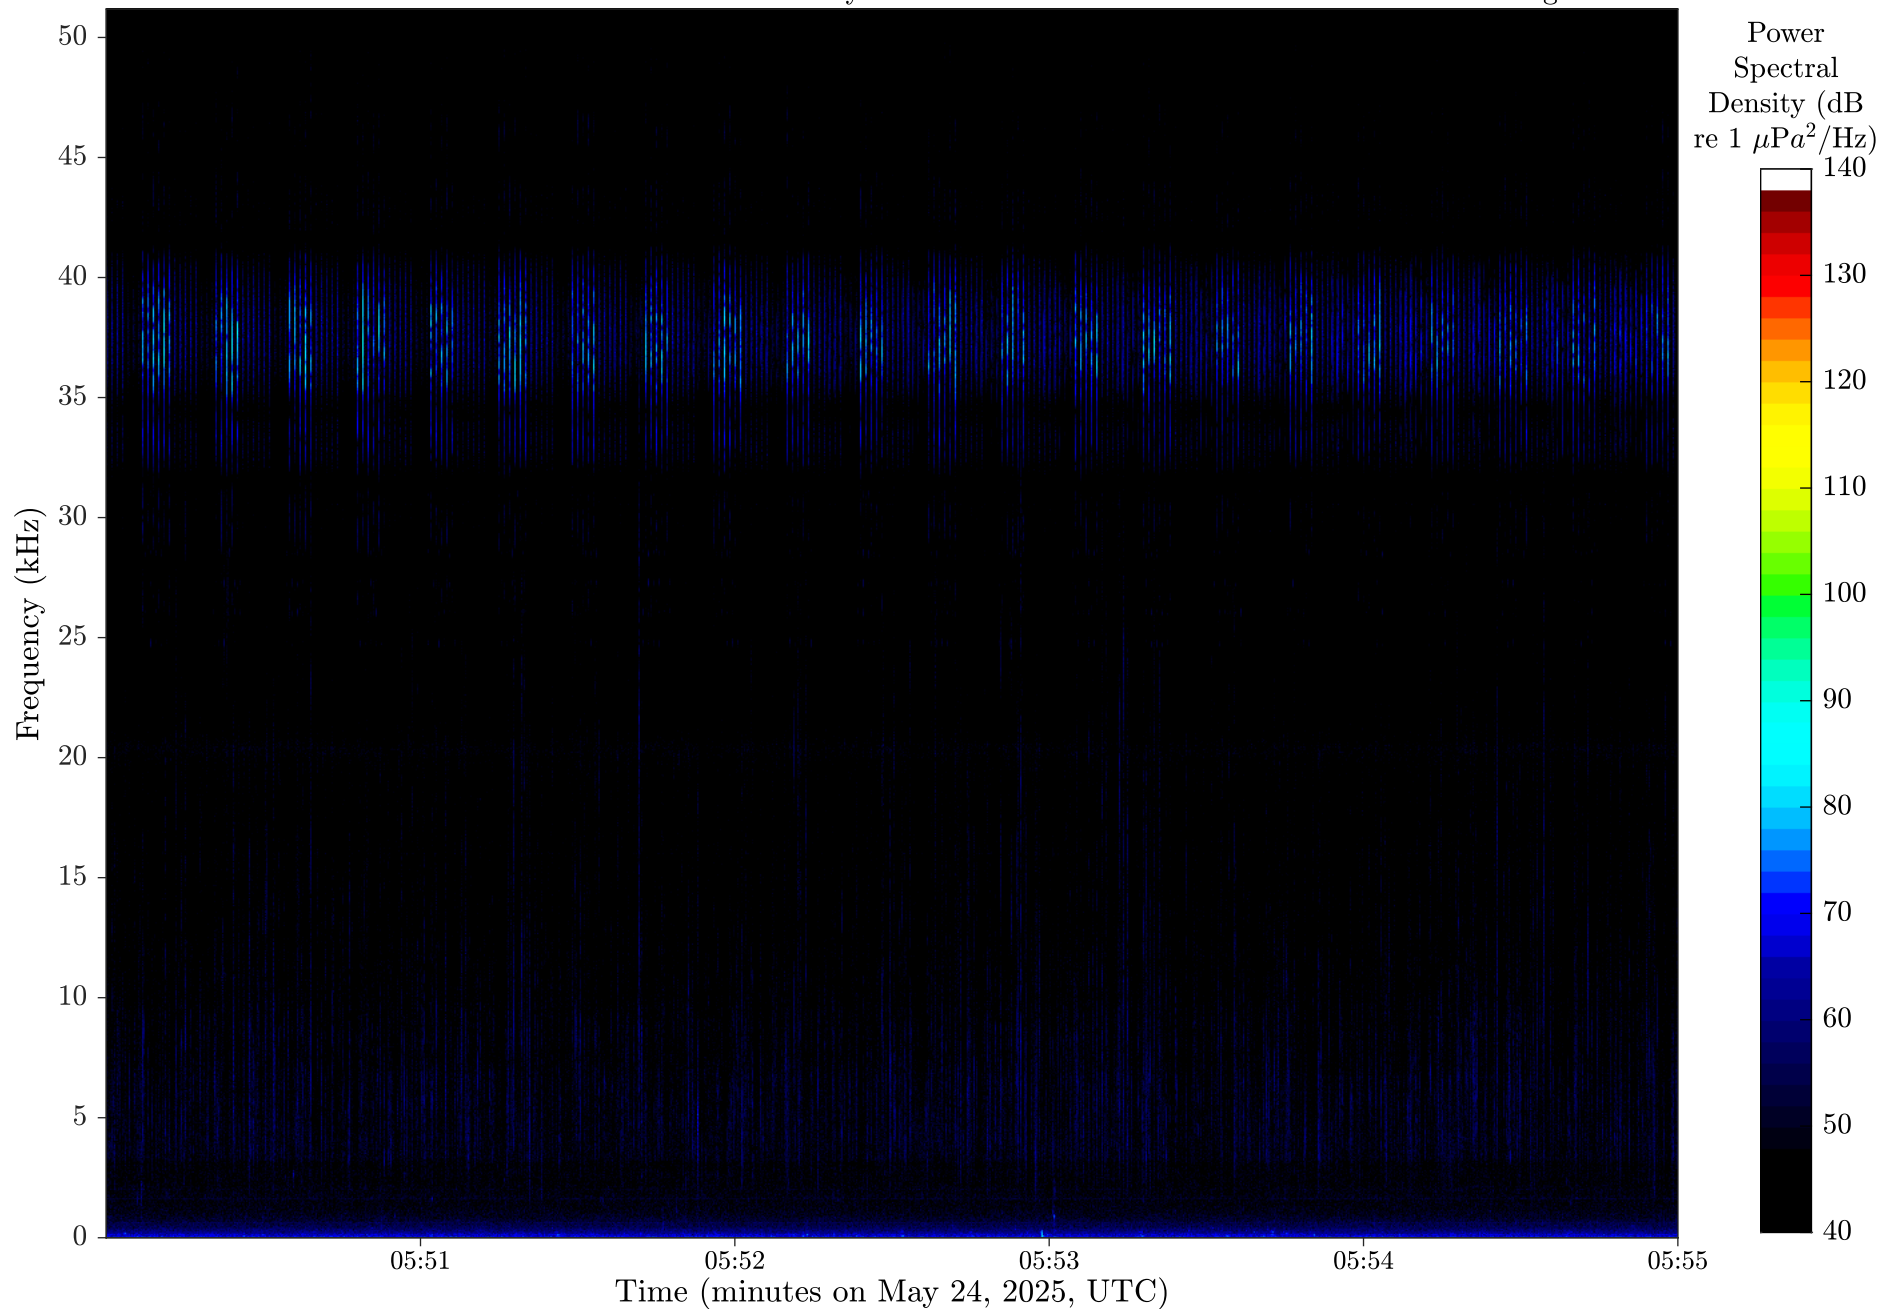

Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:24:37 UTC

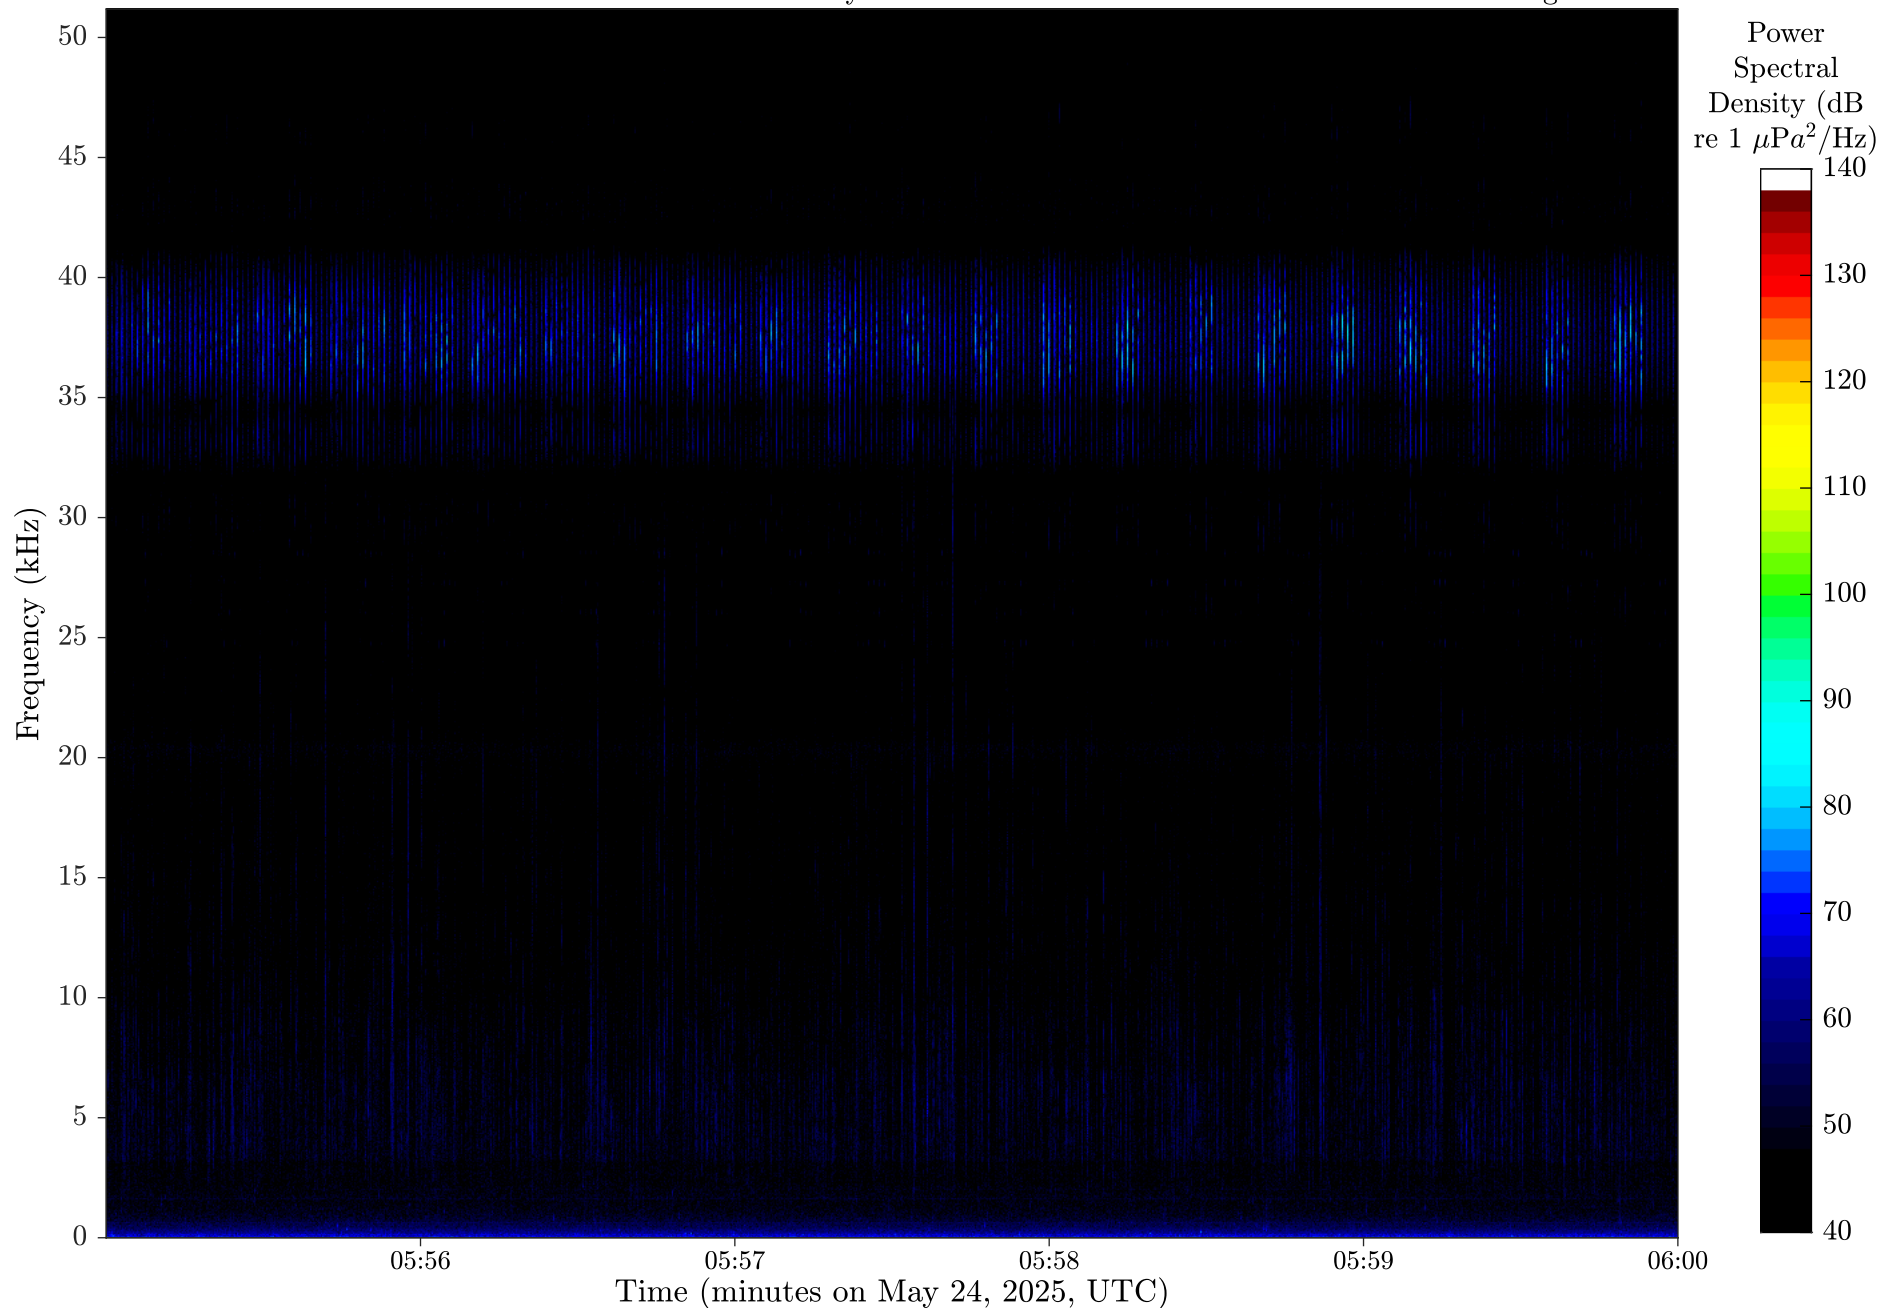

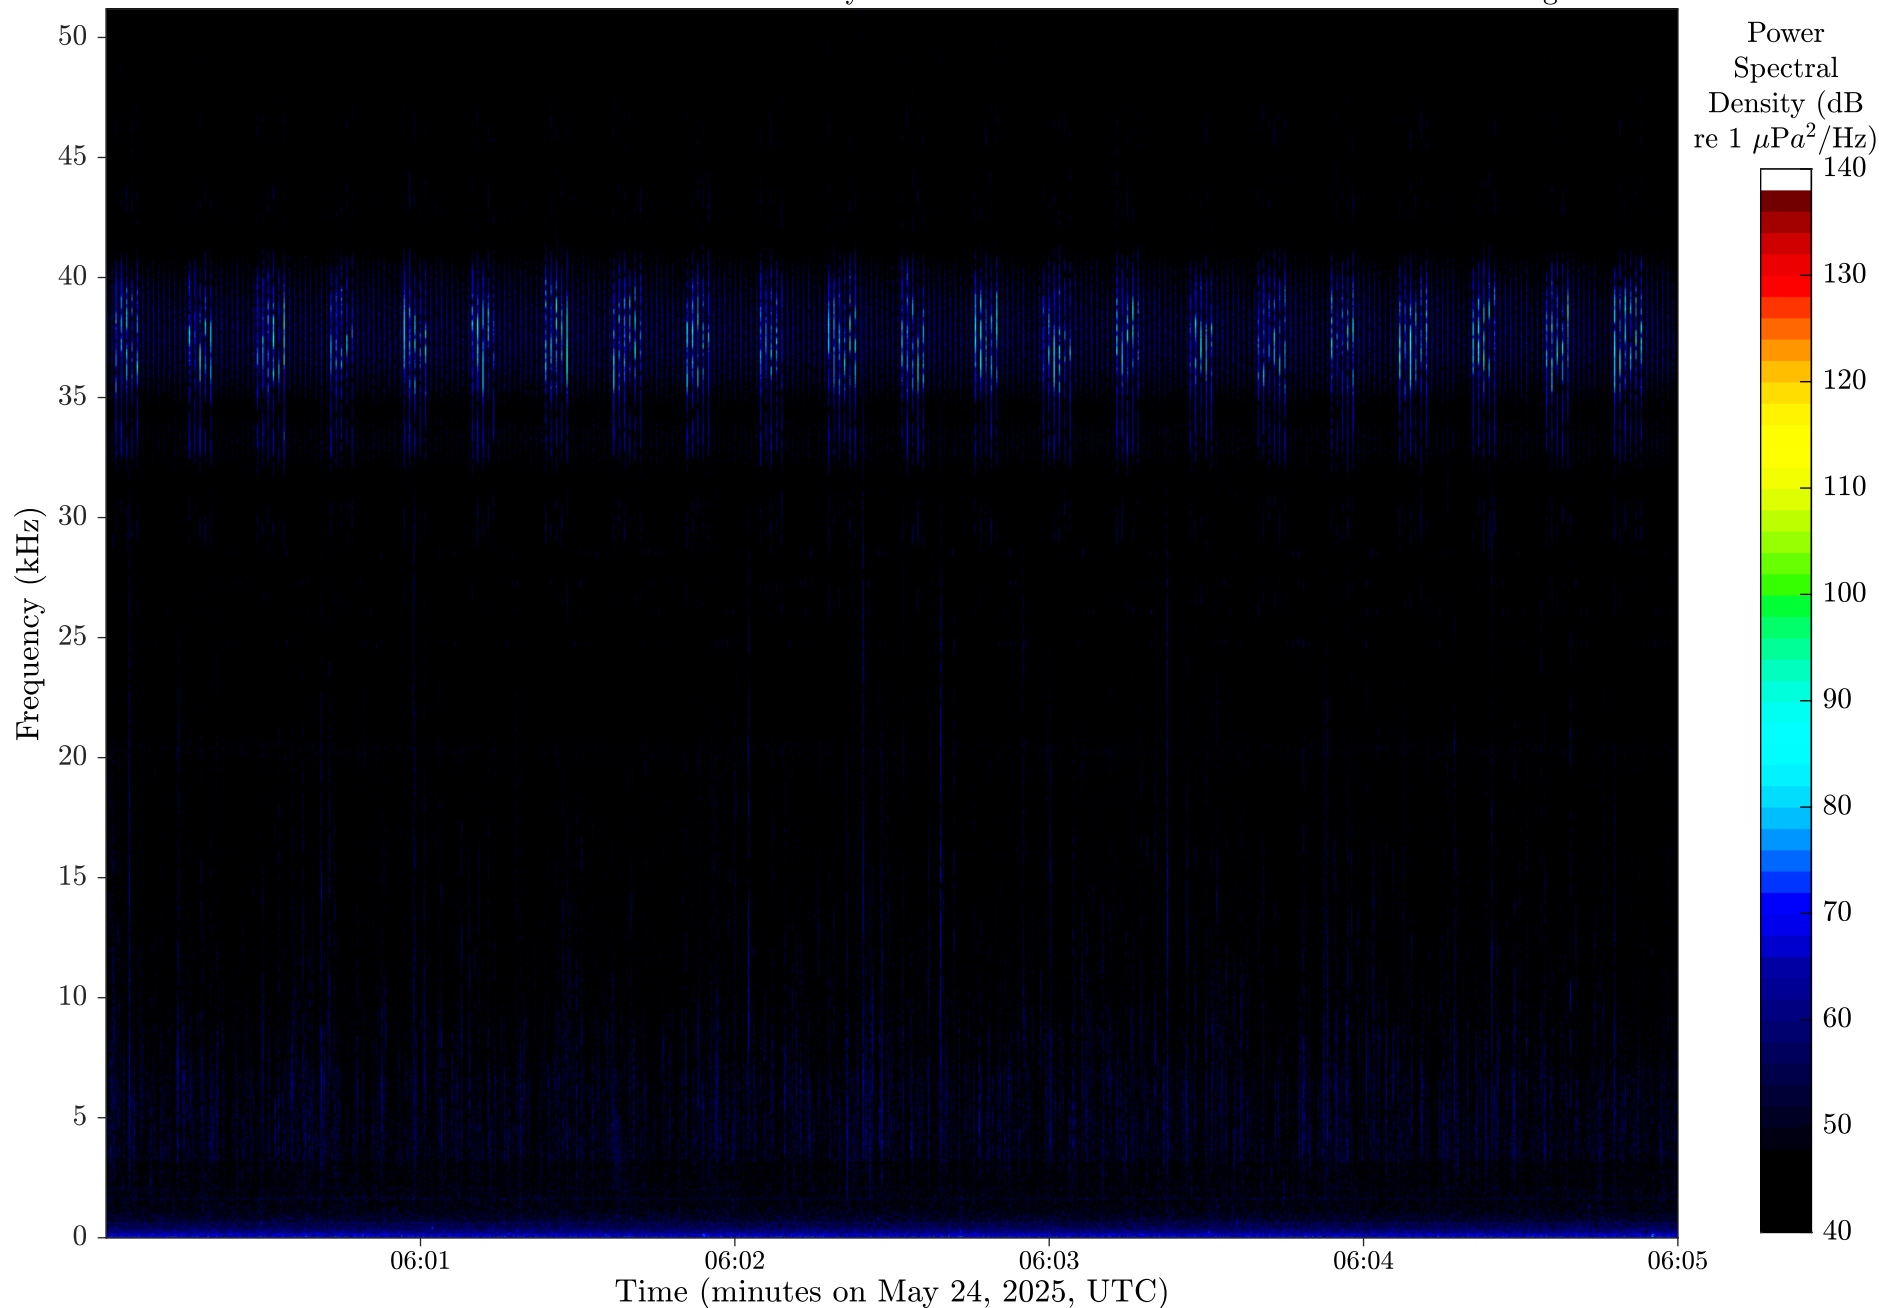


Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:24:54 UTC

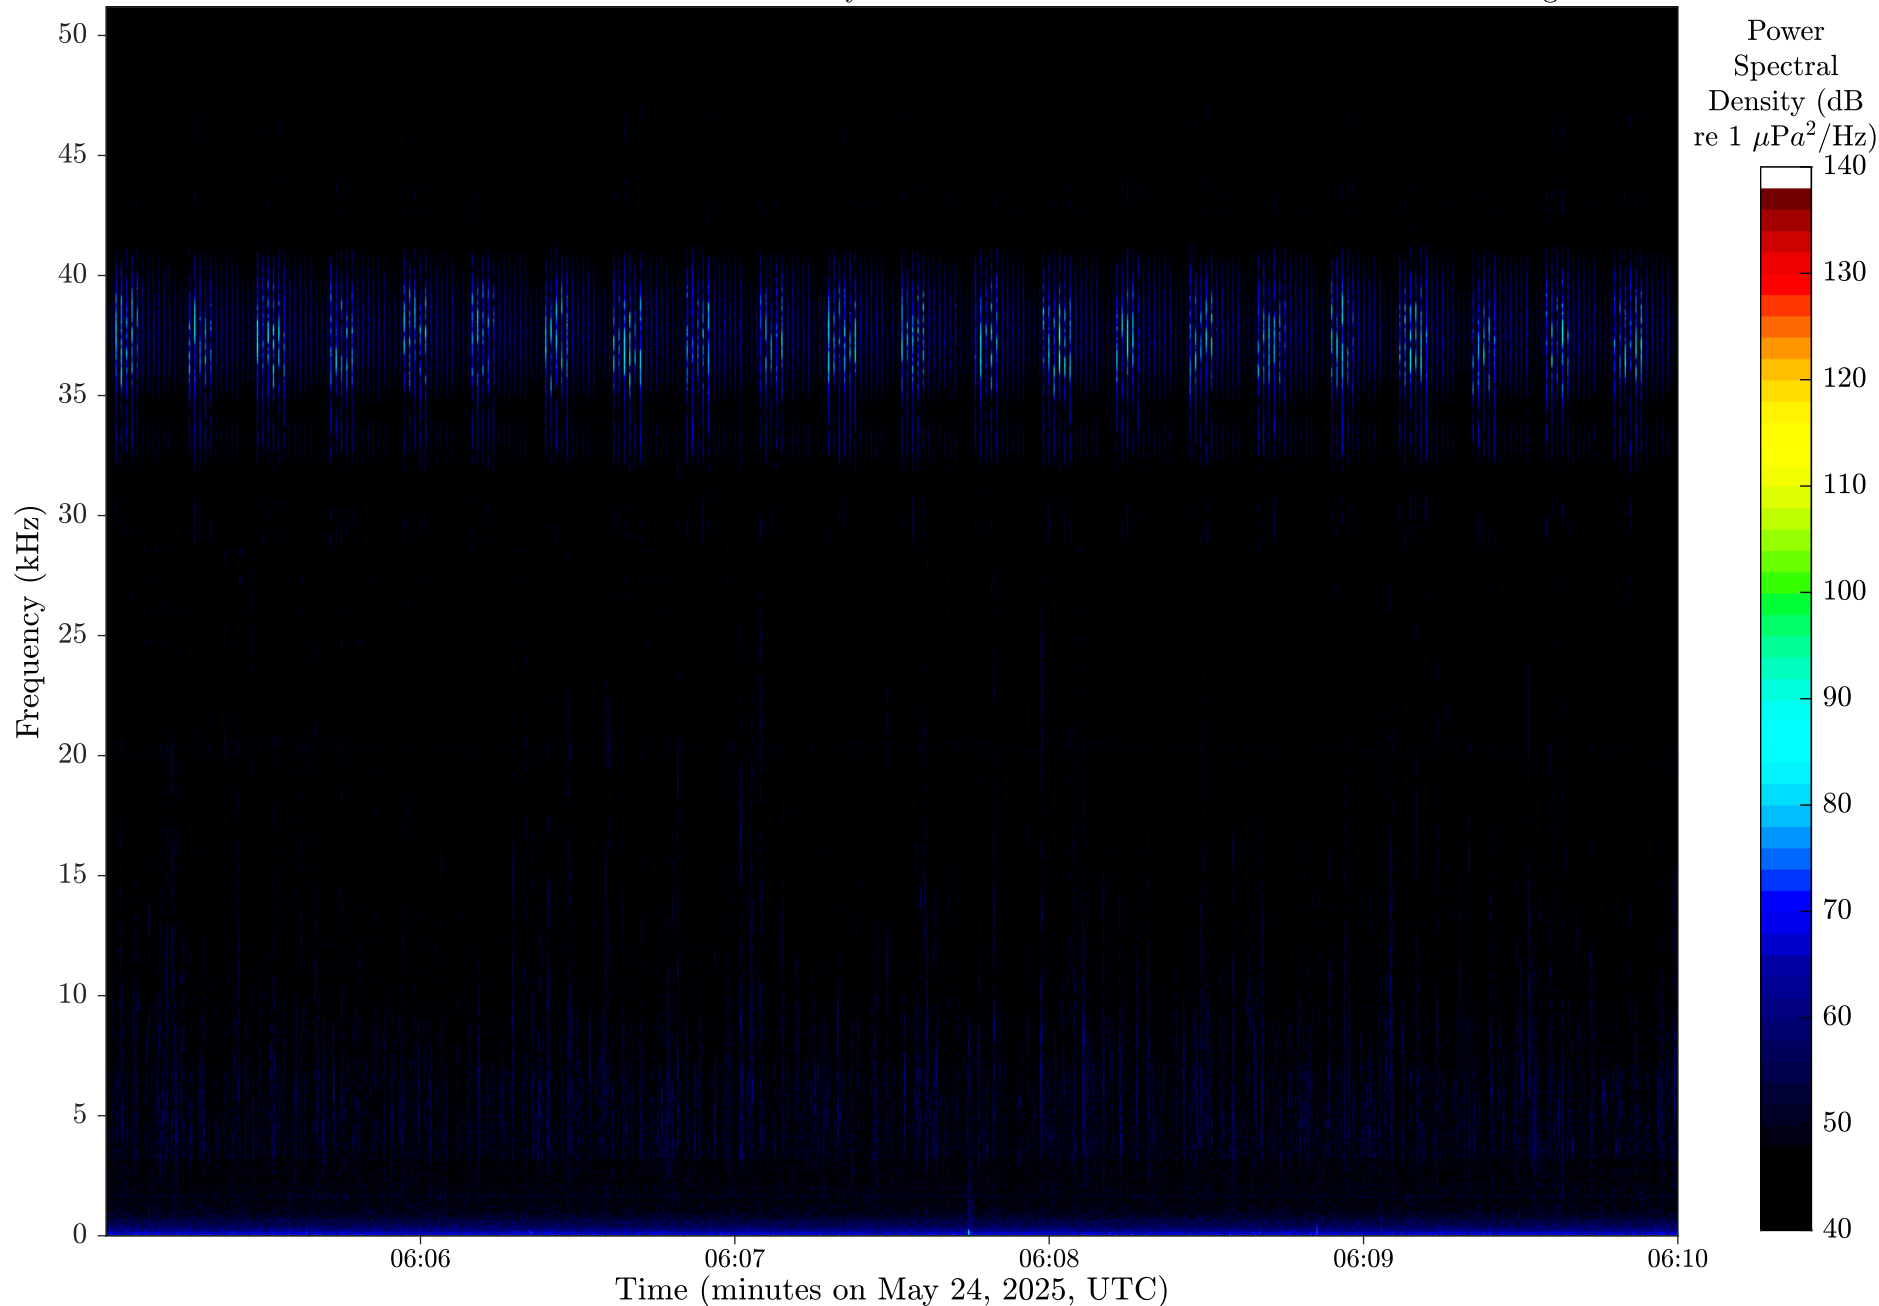

Comments: 36.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:25:03 UTC

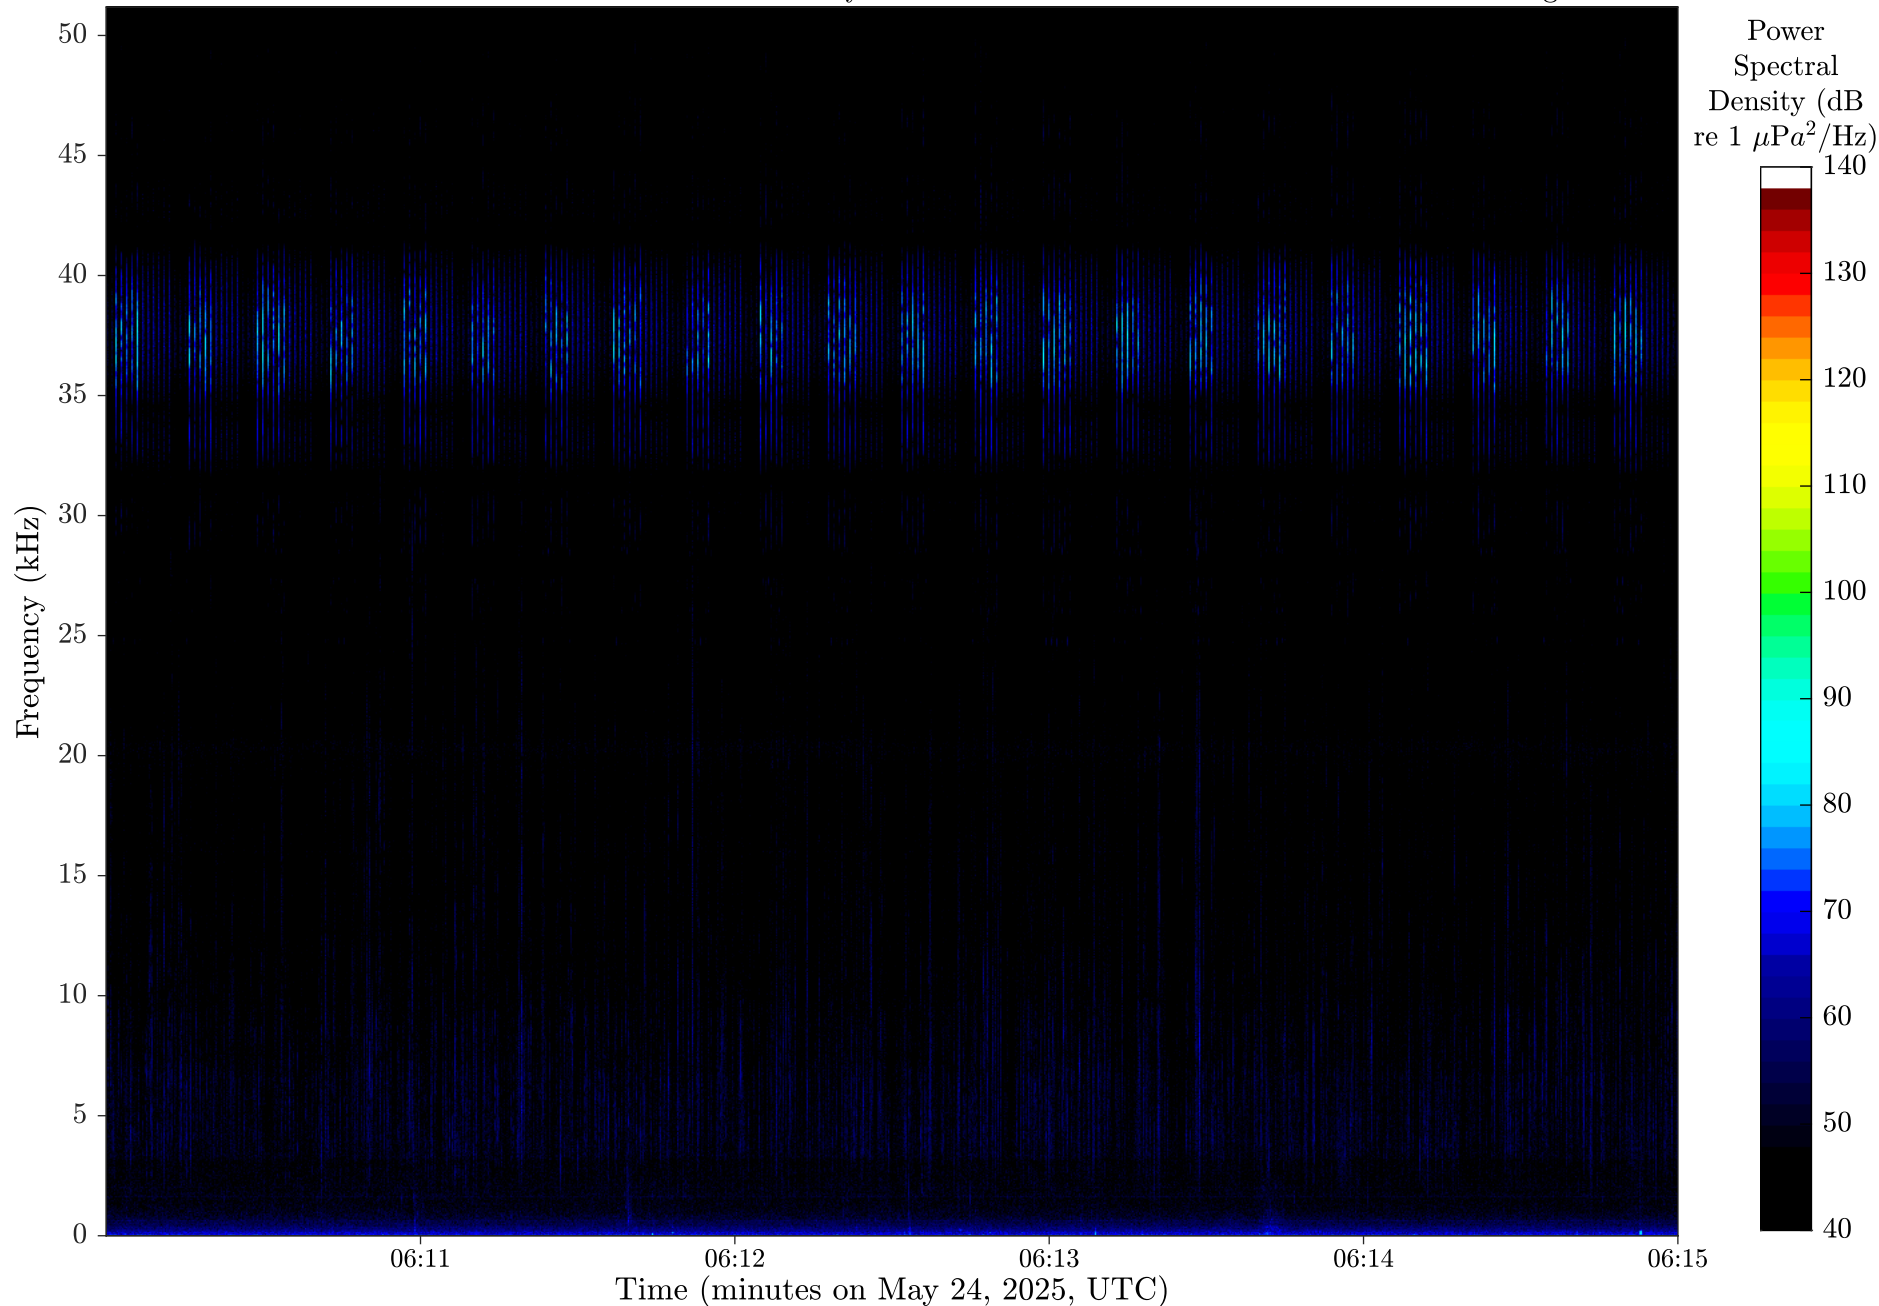

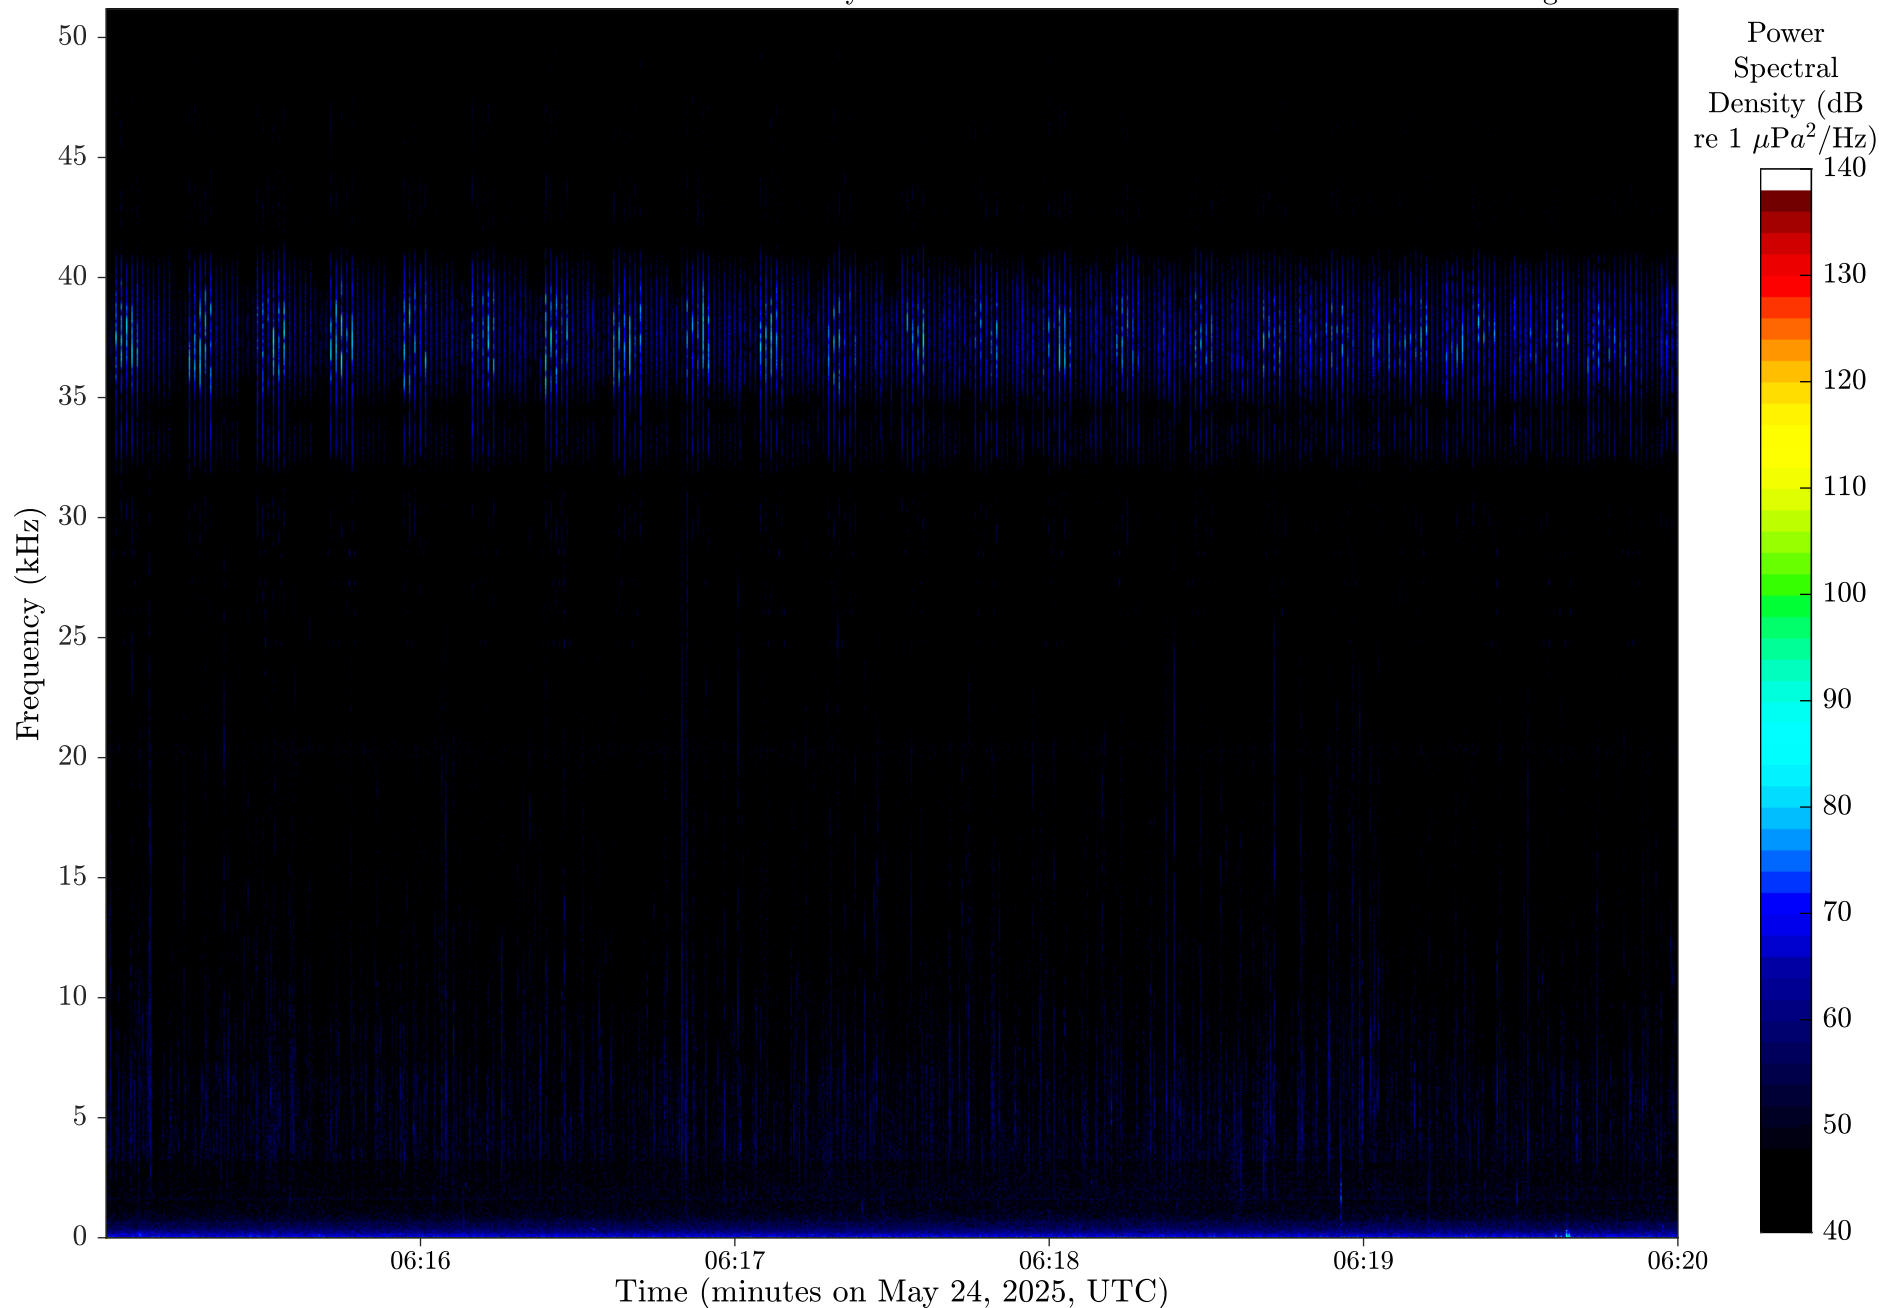


Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:20 UTC

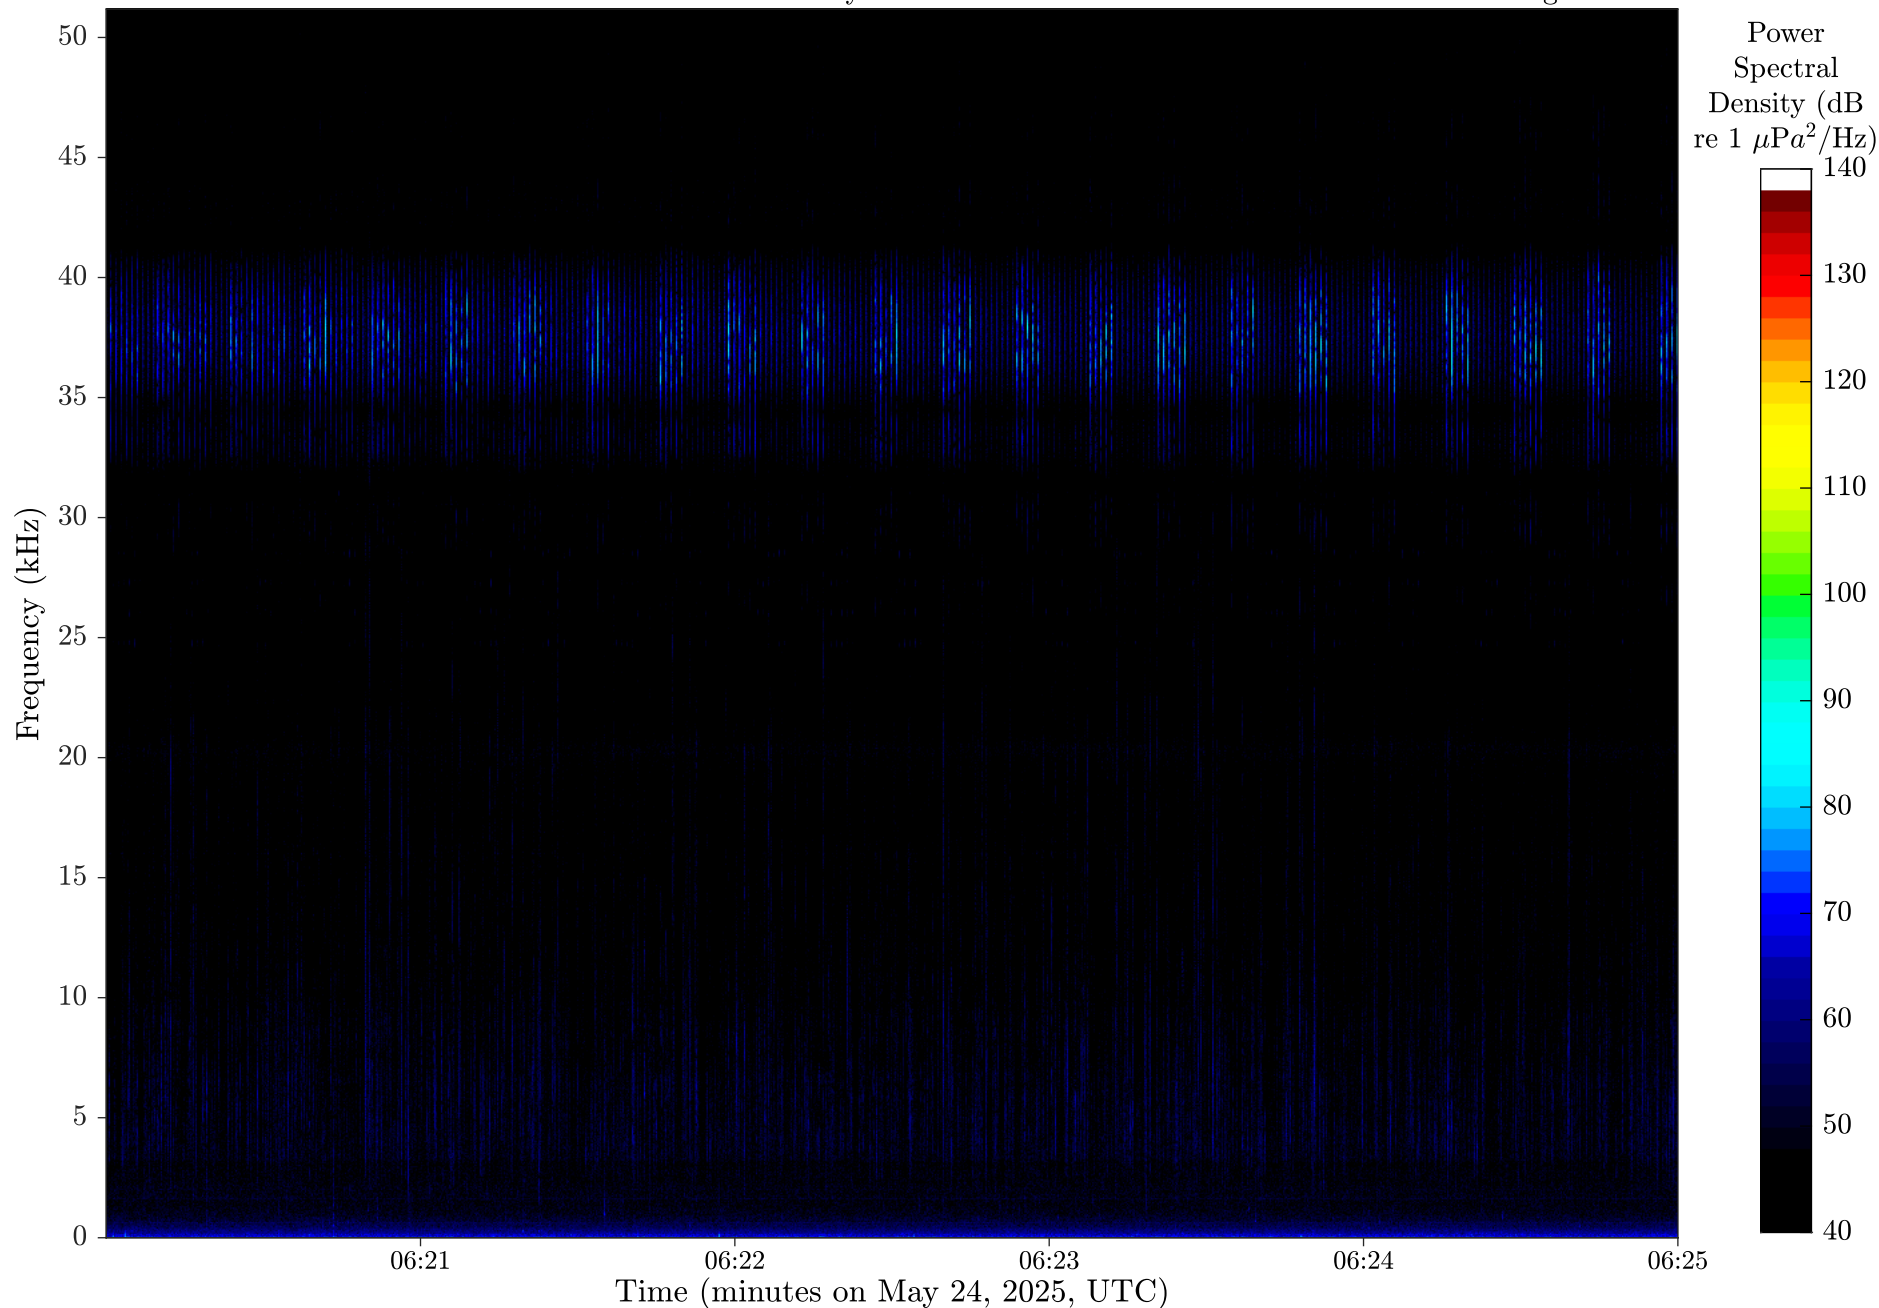


Comments: 35.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:28 UTC

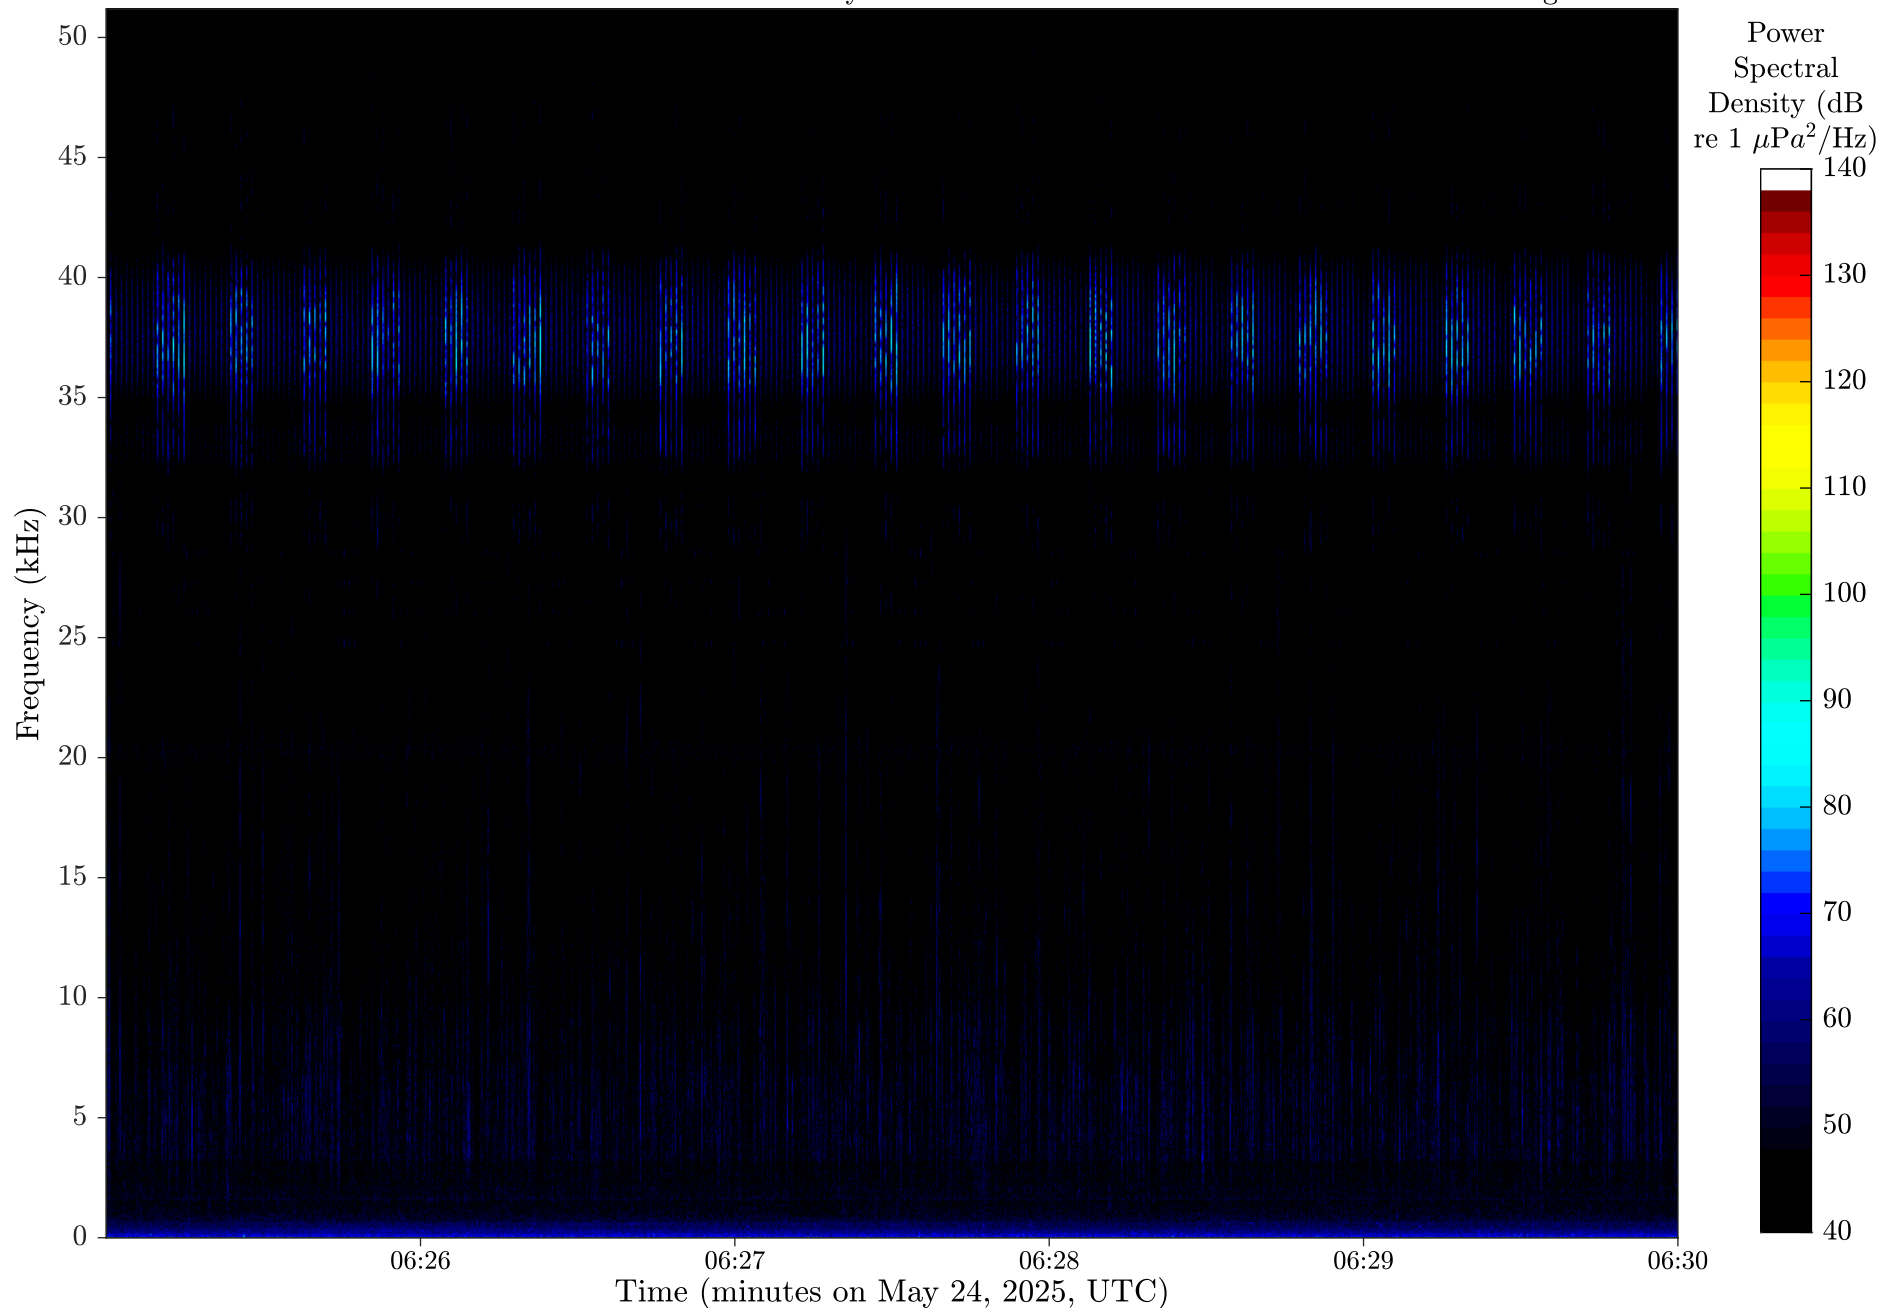


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:36 UTC

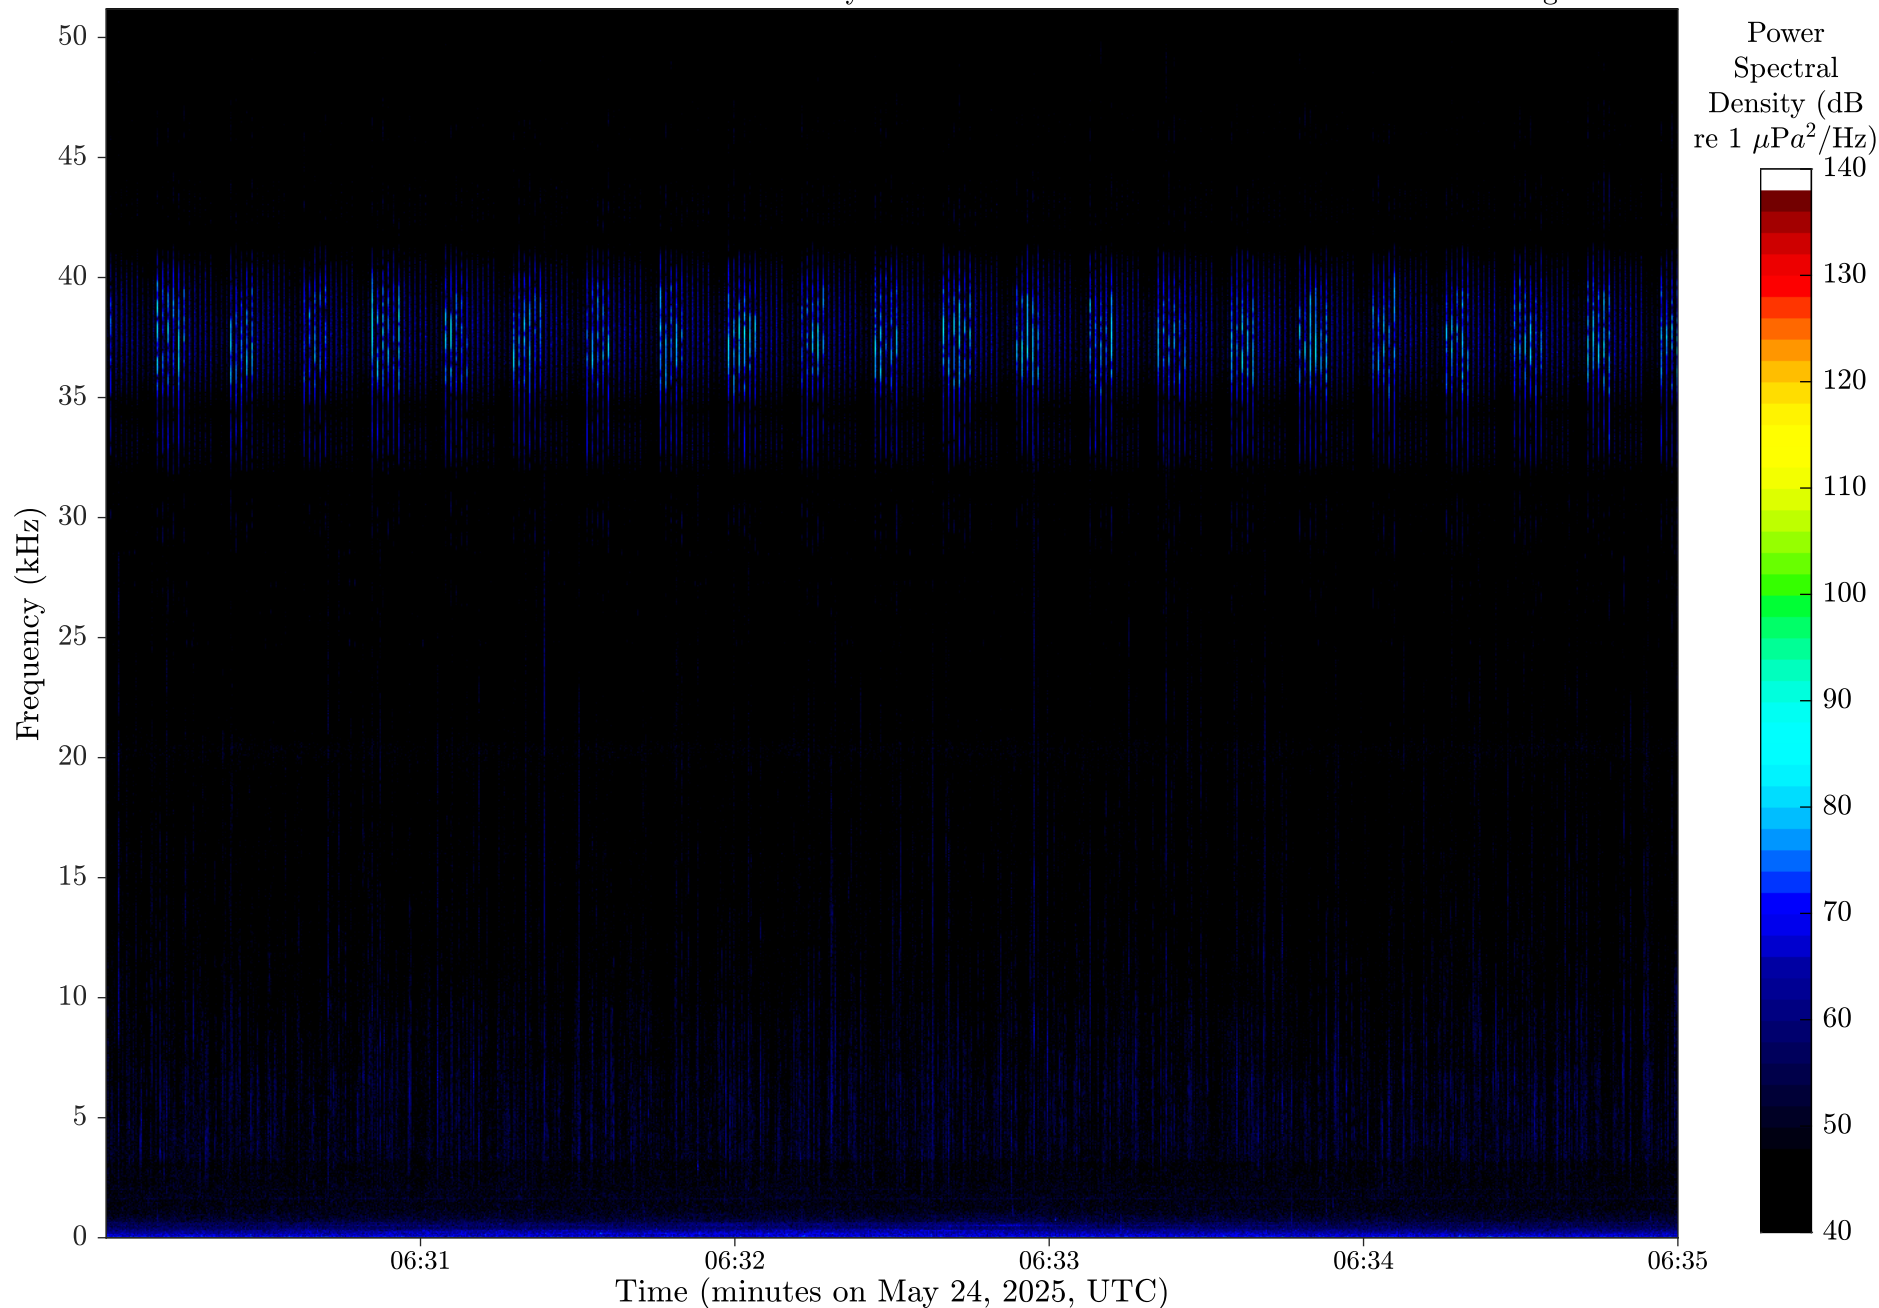


Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:25:45 UTC

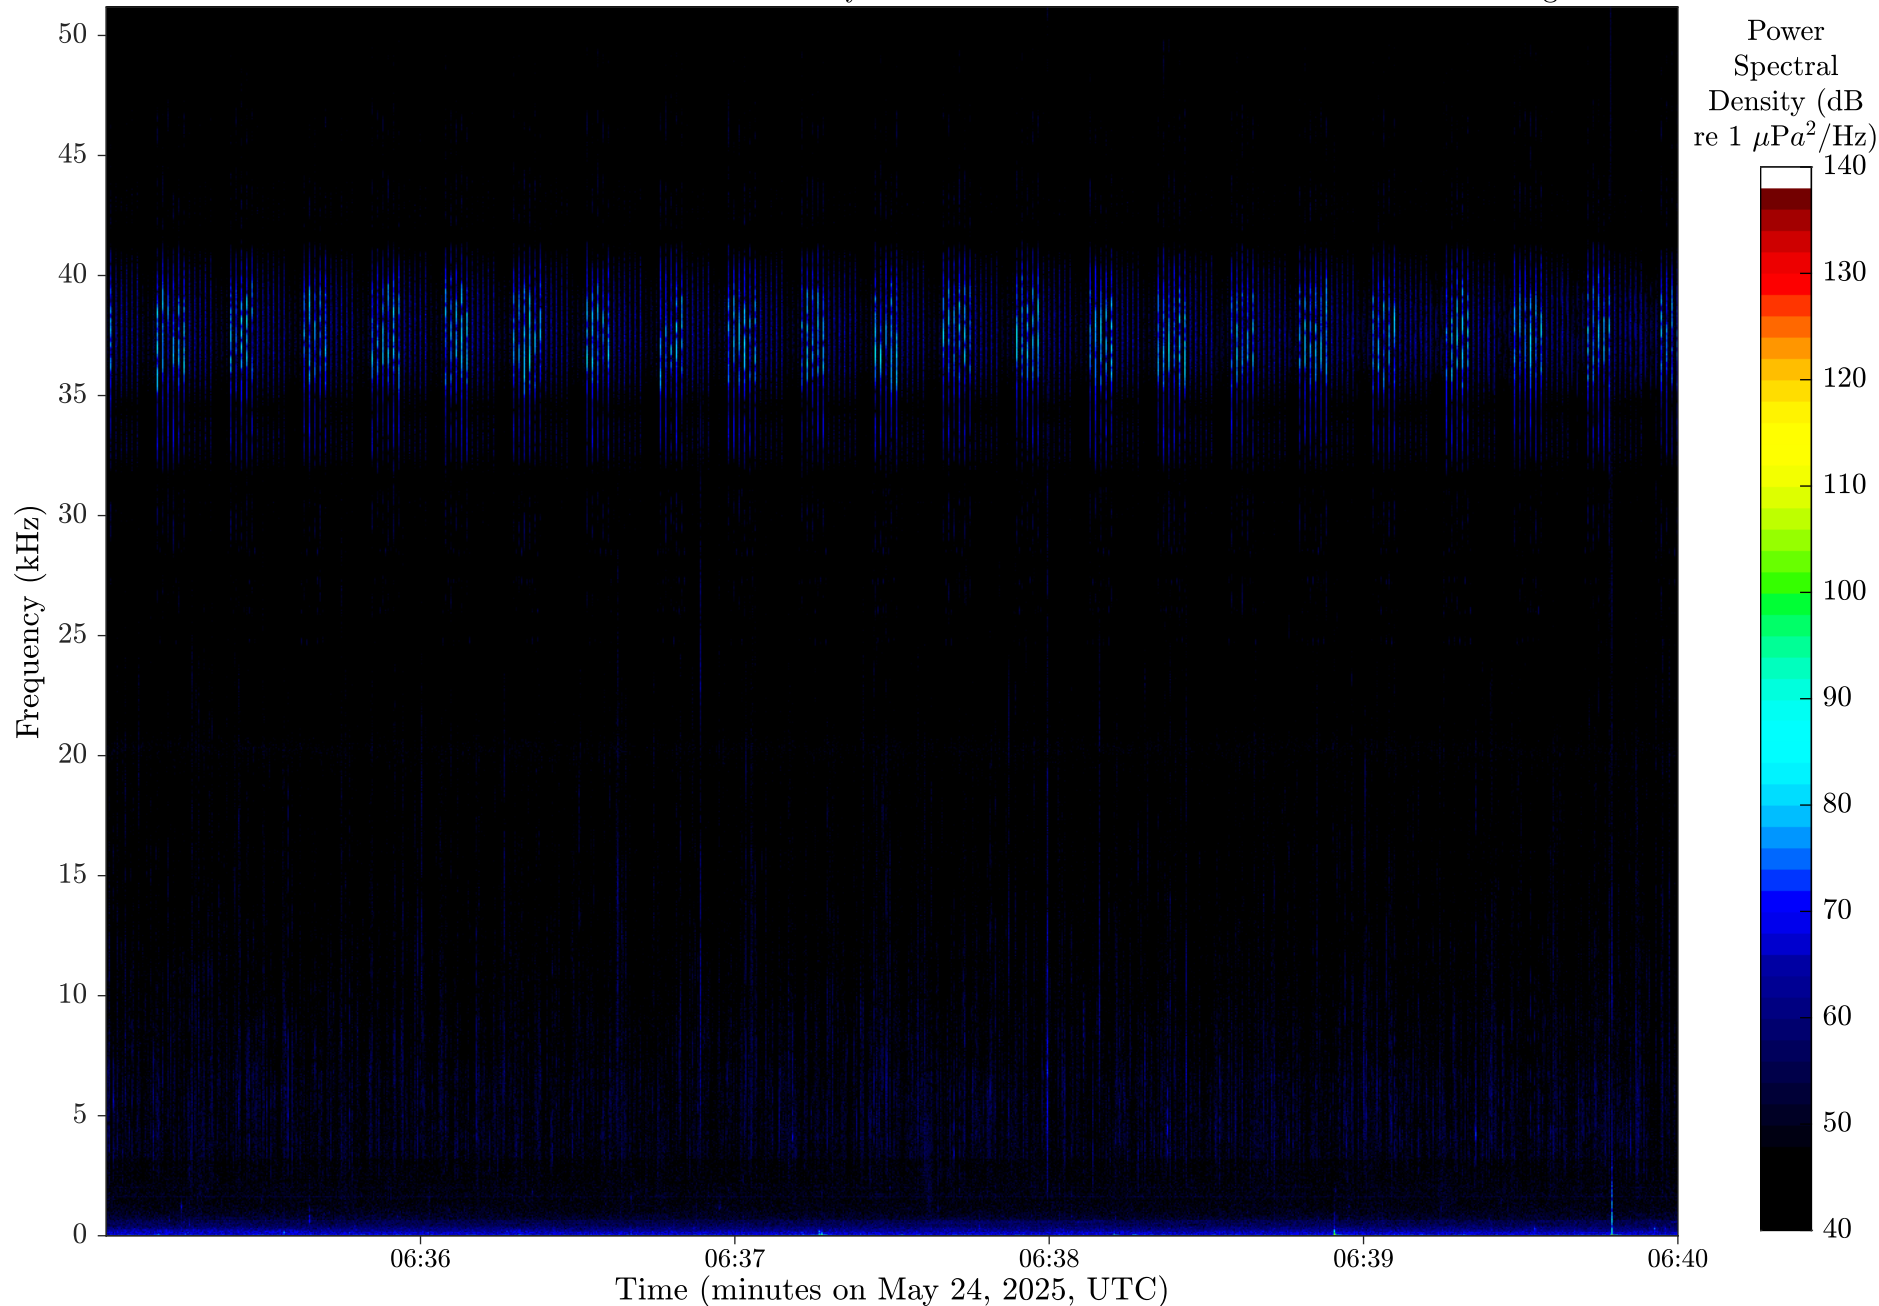



Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:53 UTC

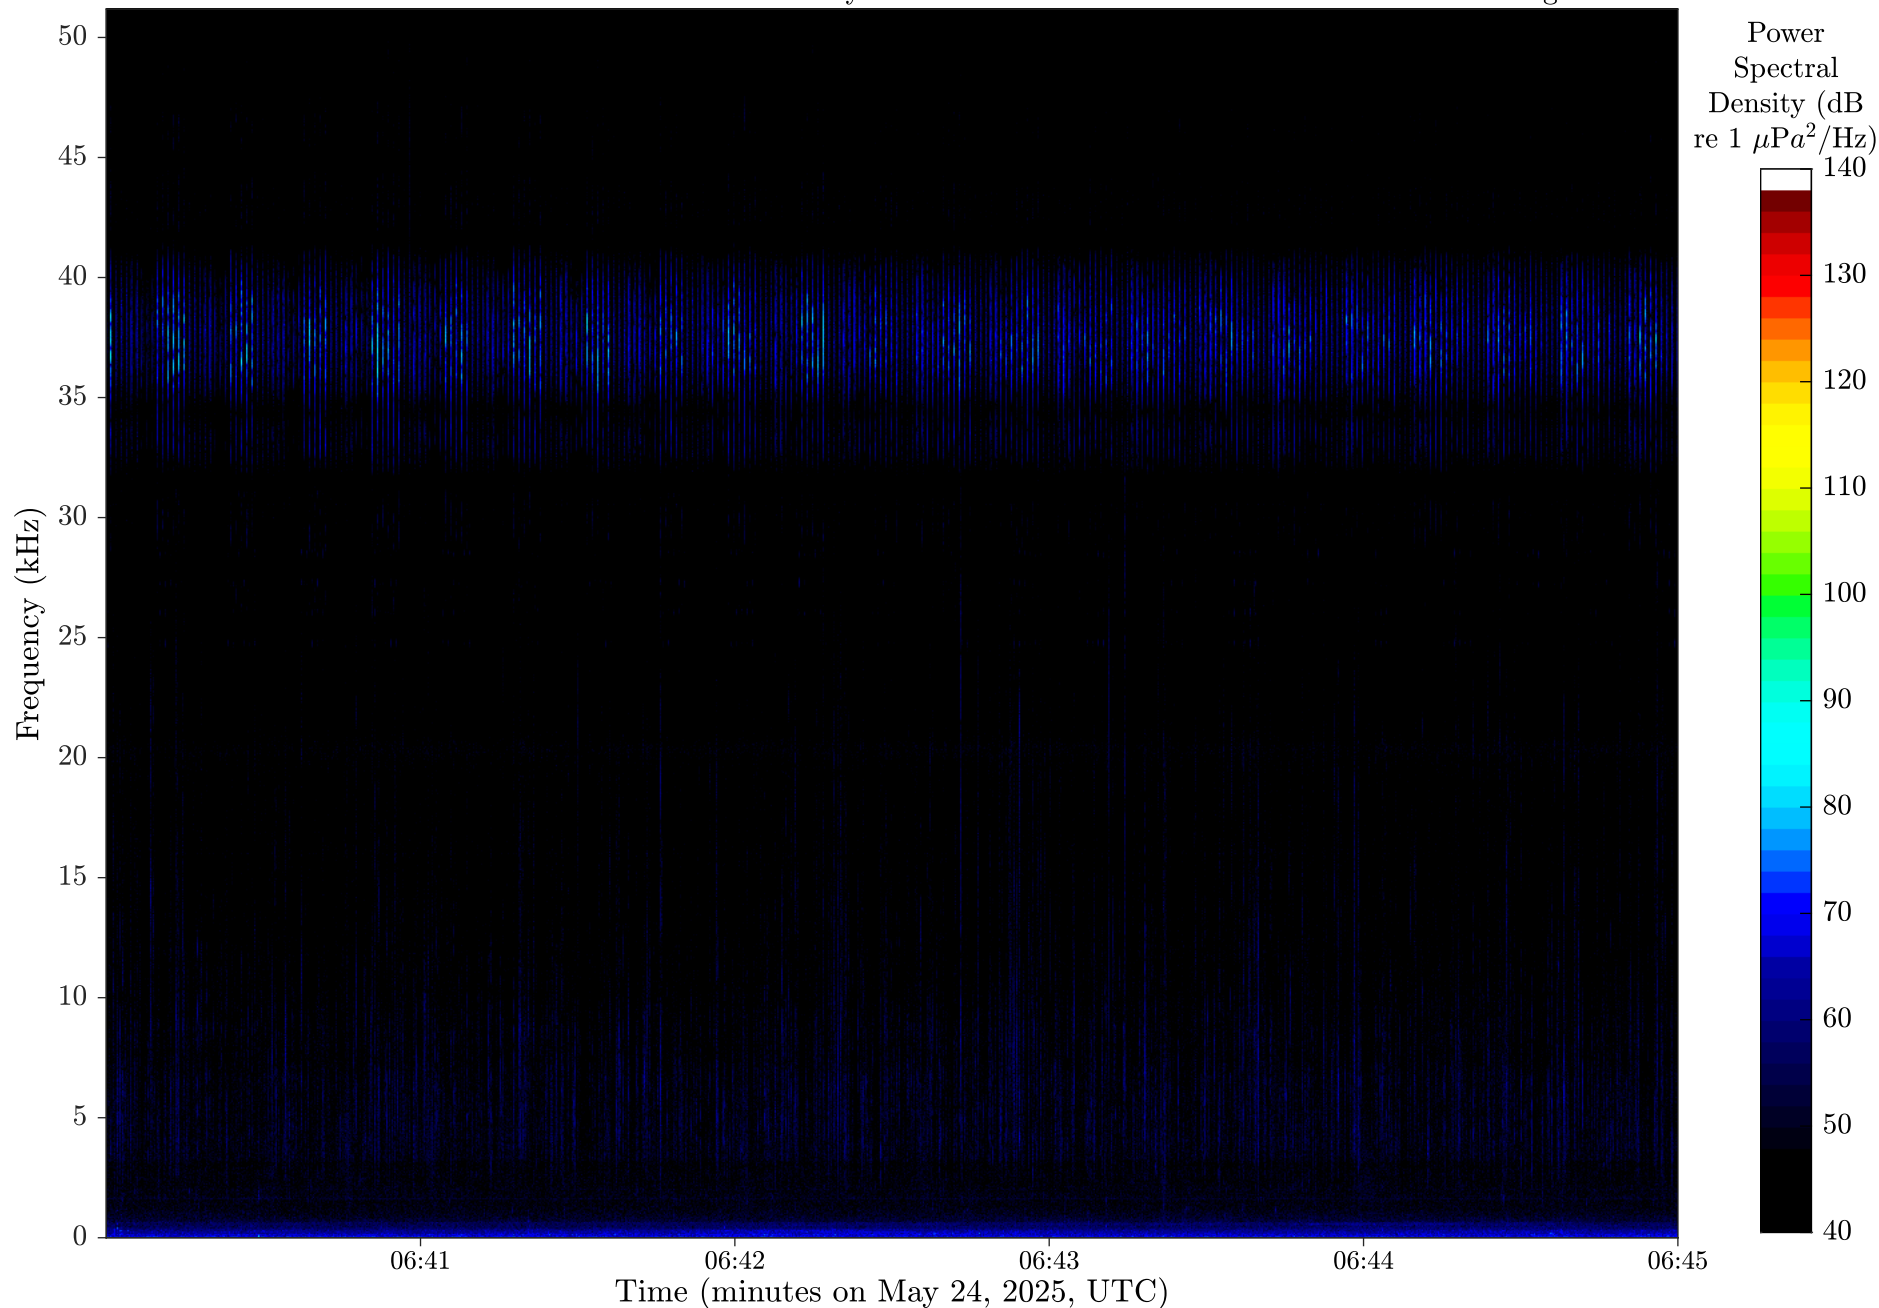

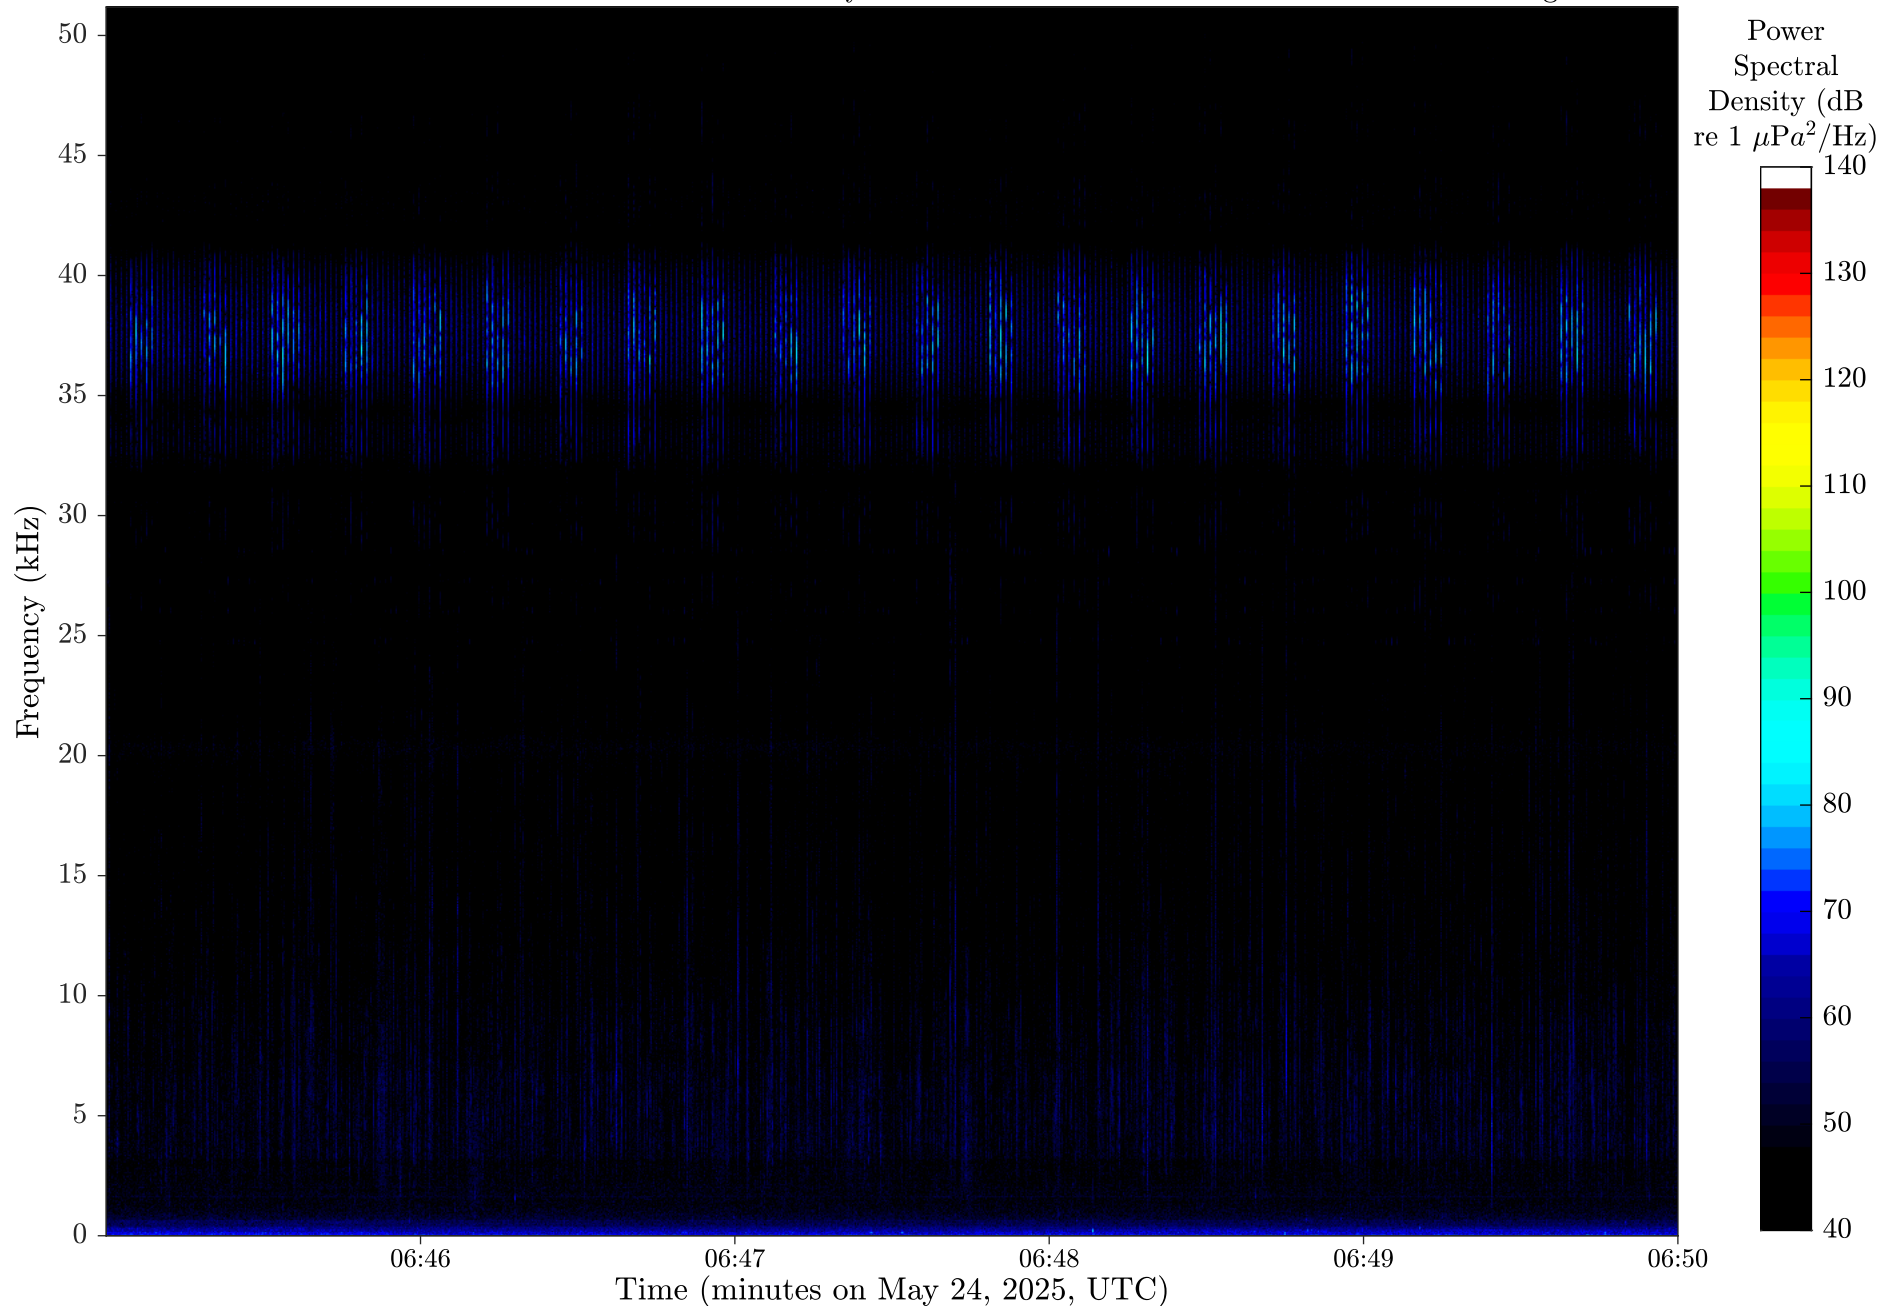


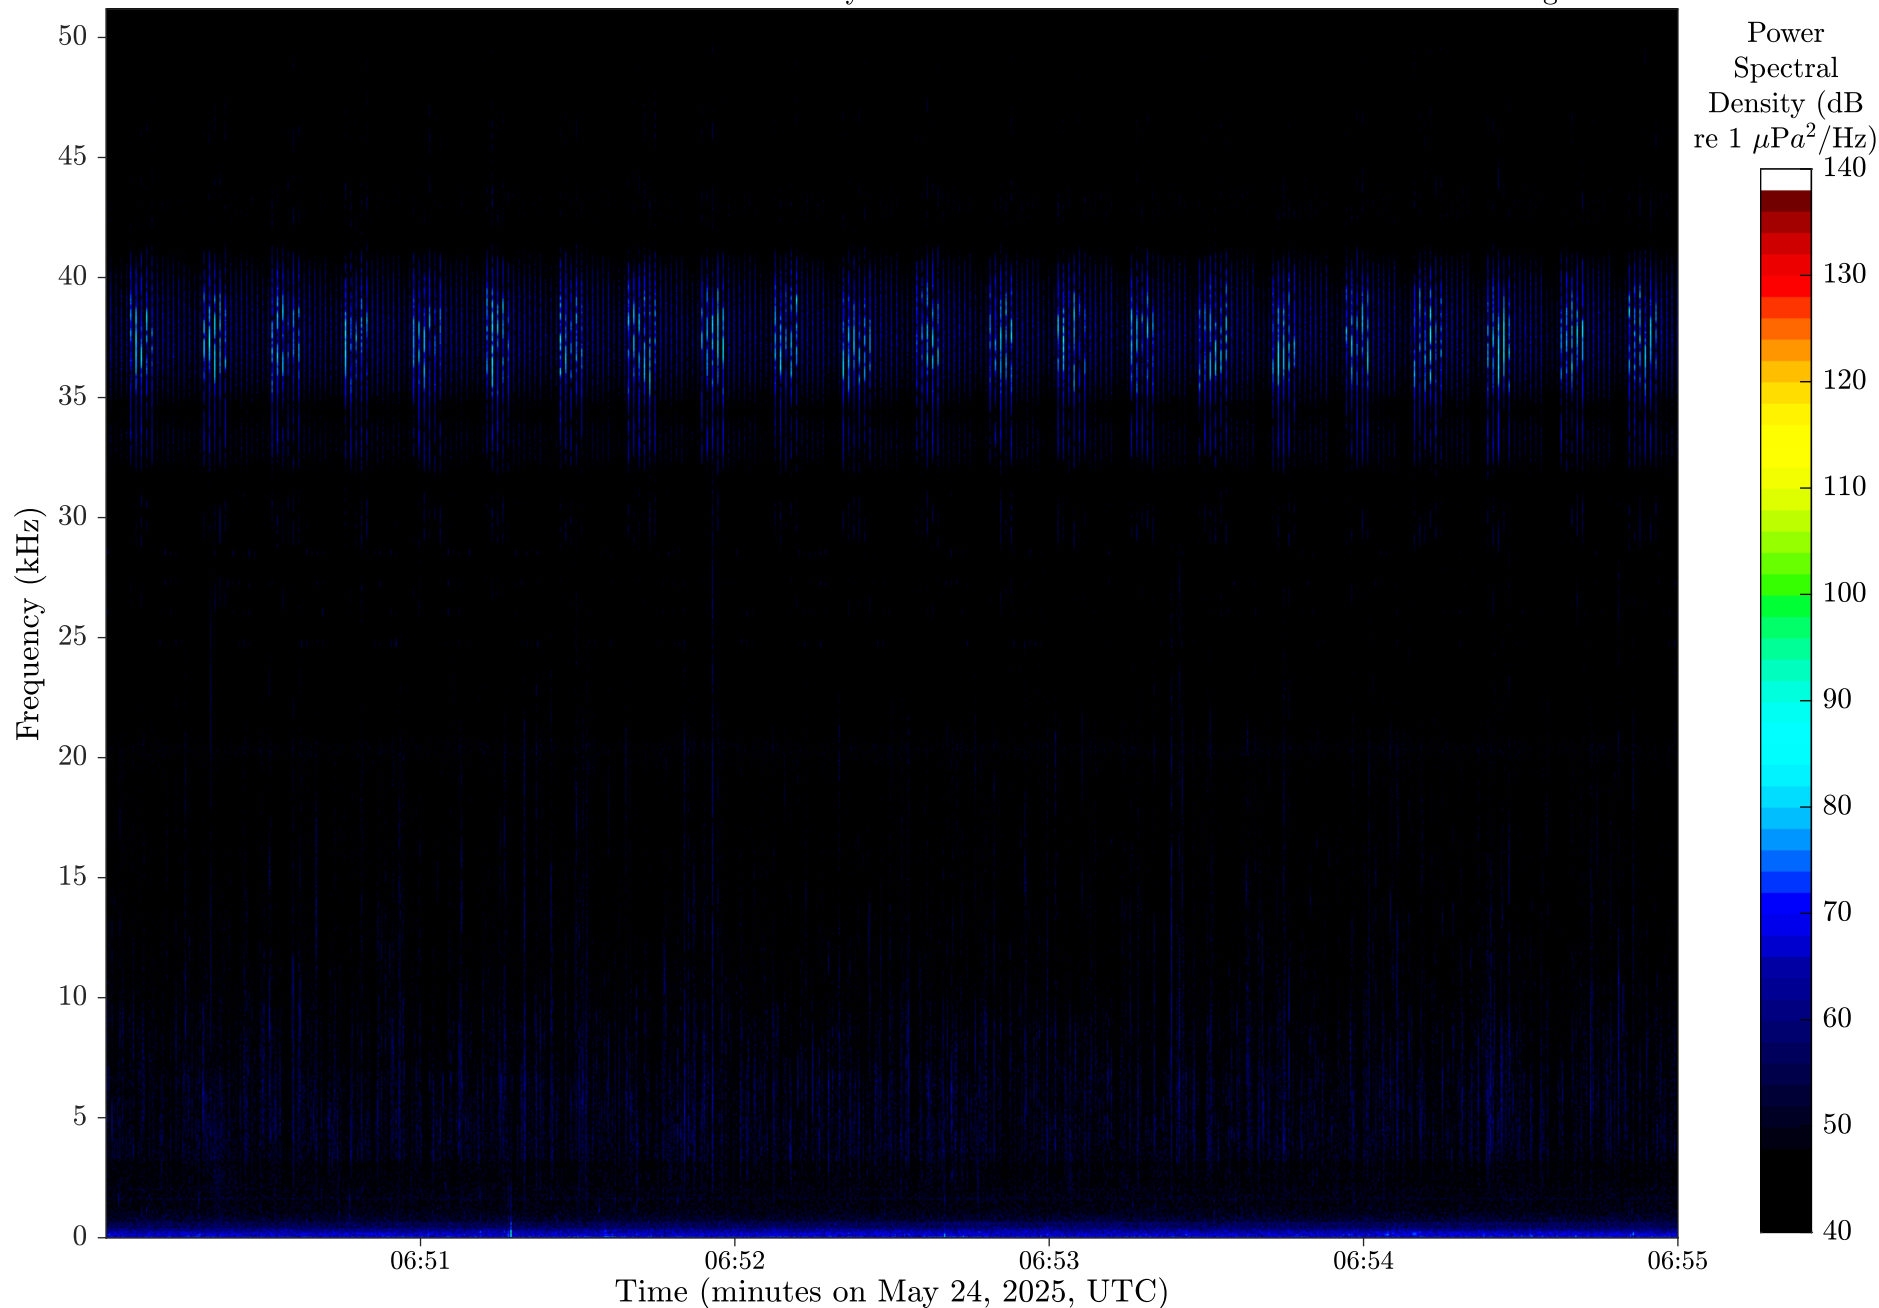

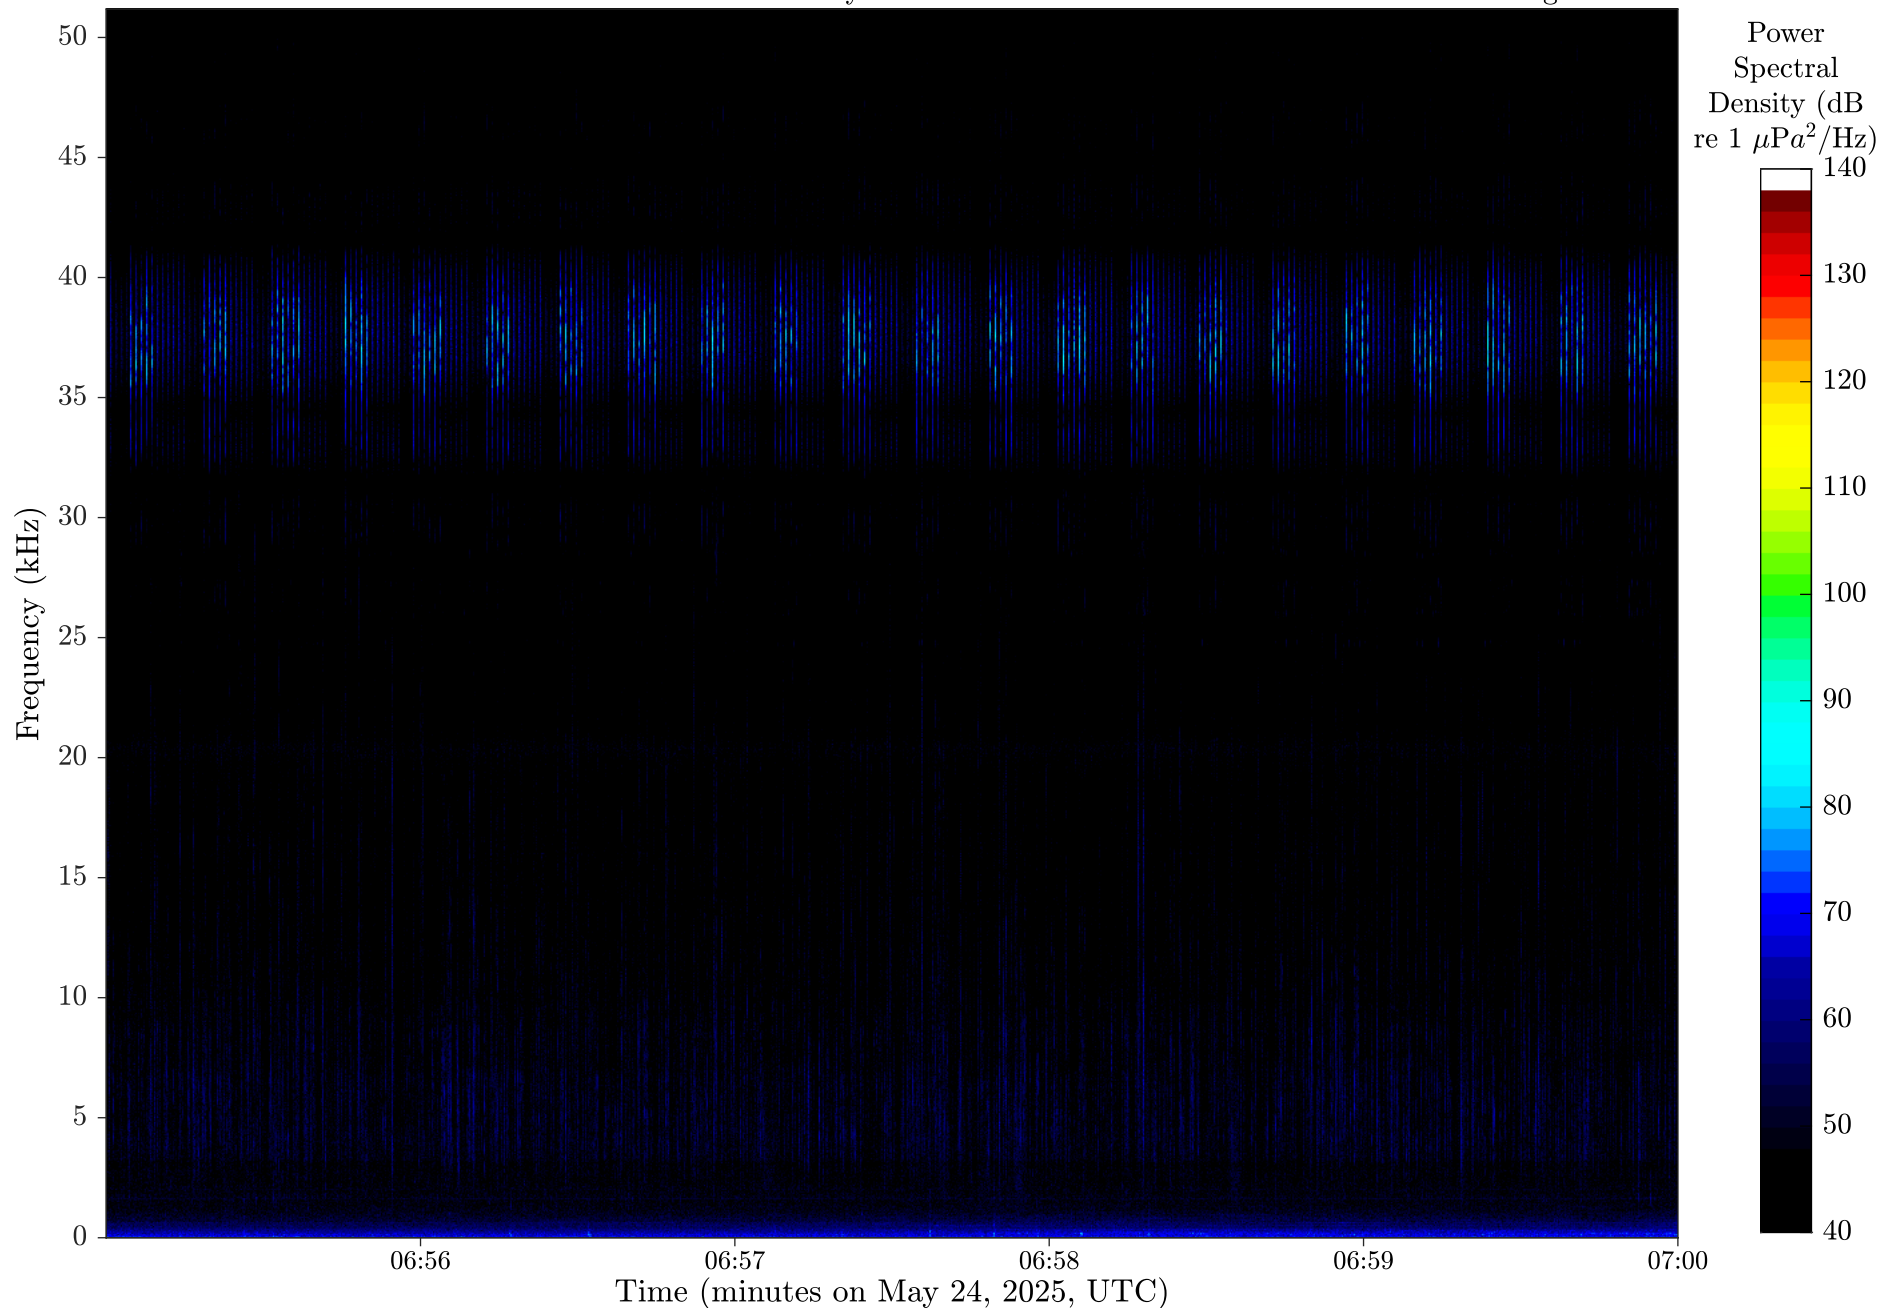


Comments: 36.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:26:27 UTC

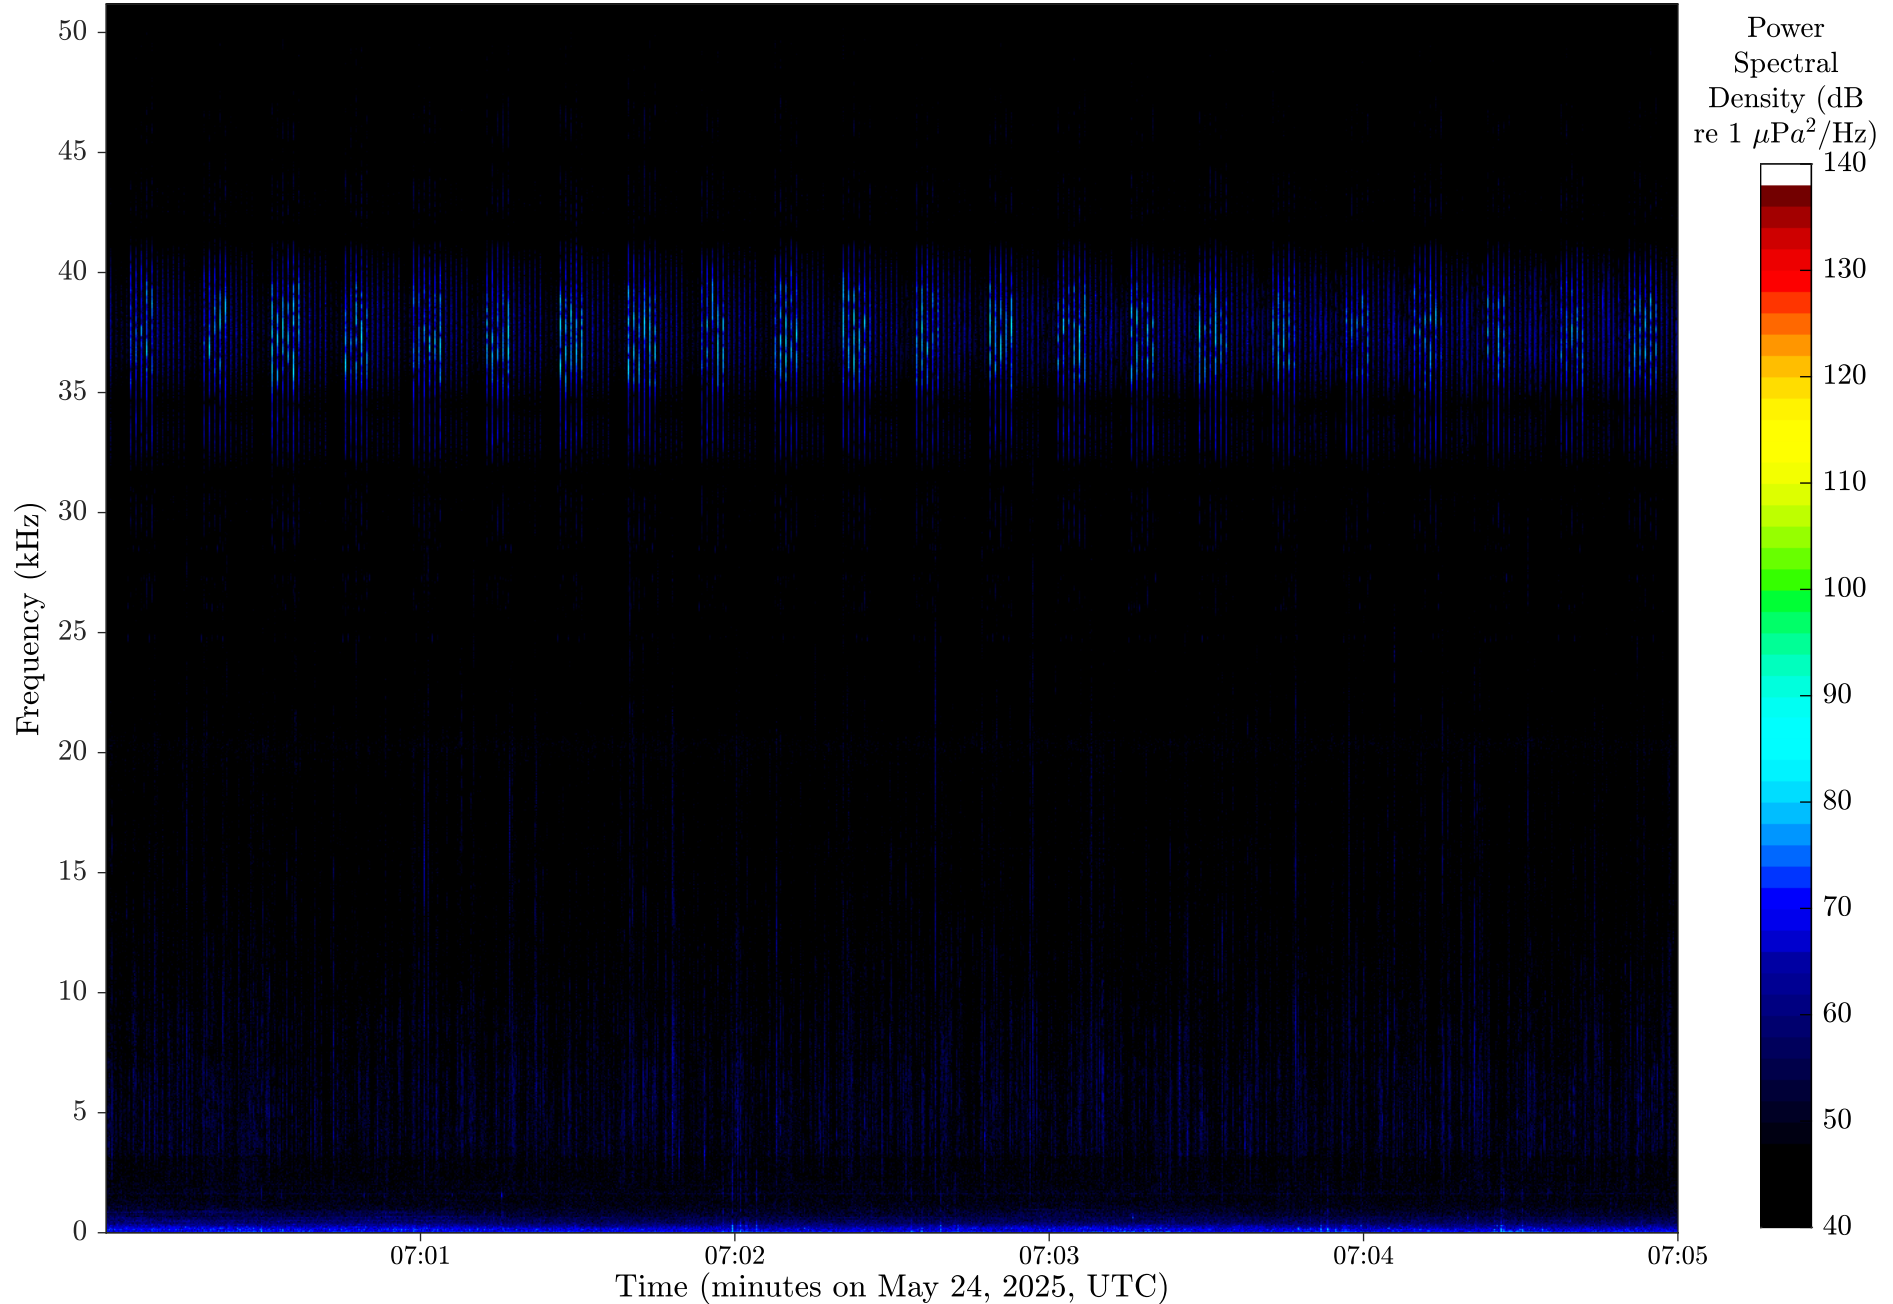

Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:26:35 UTC

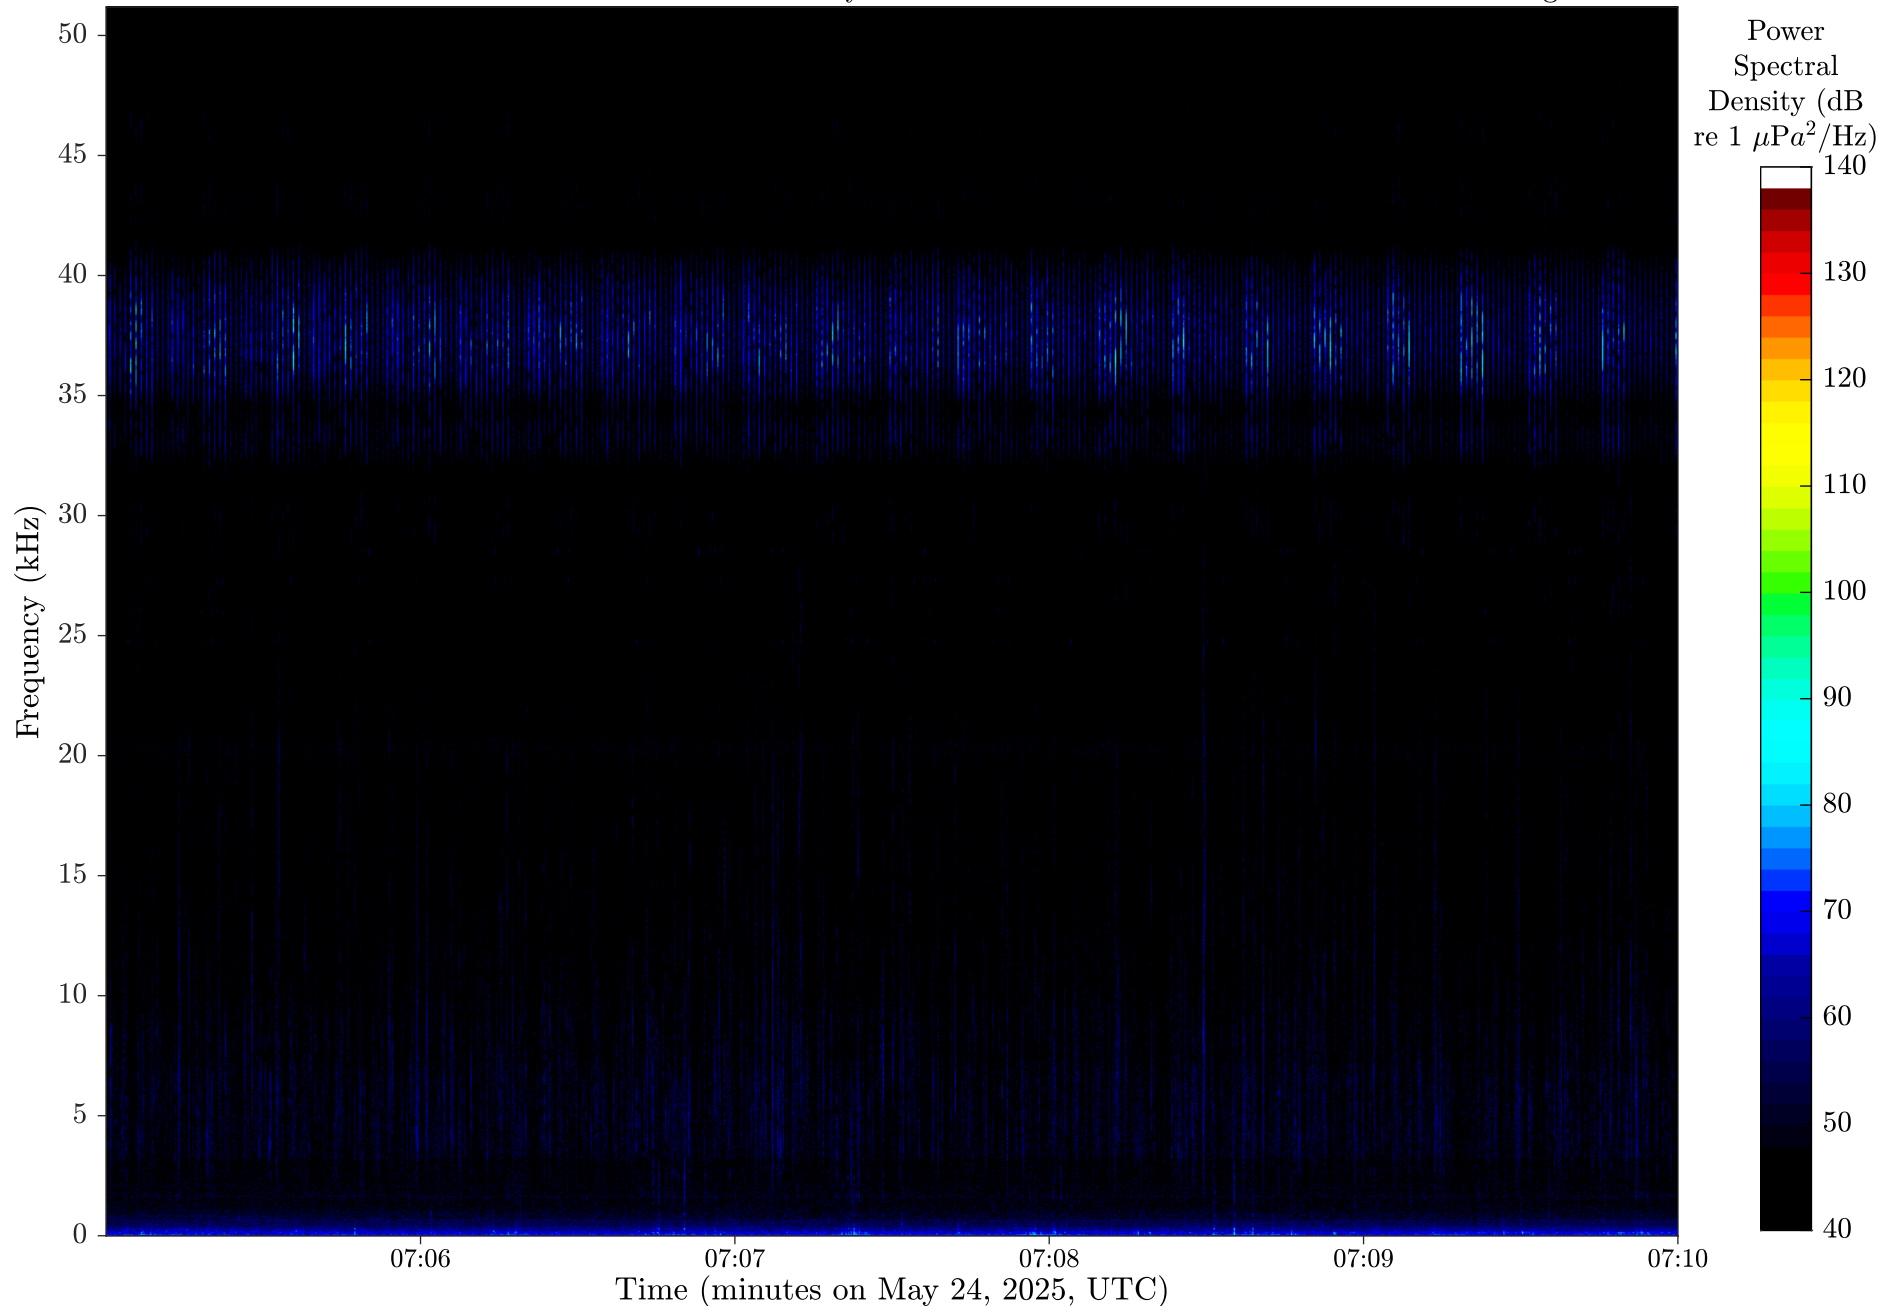


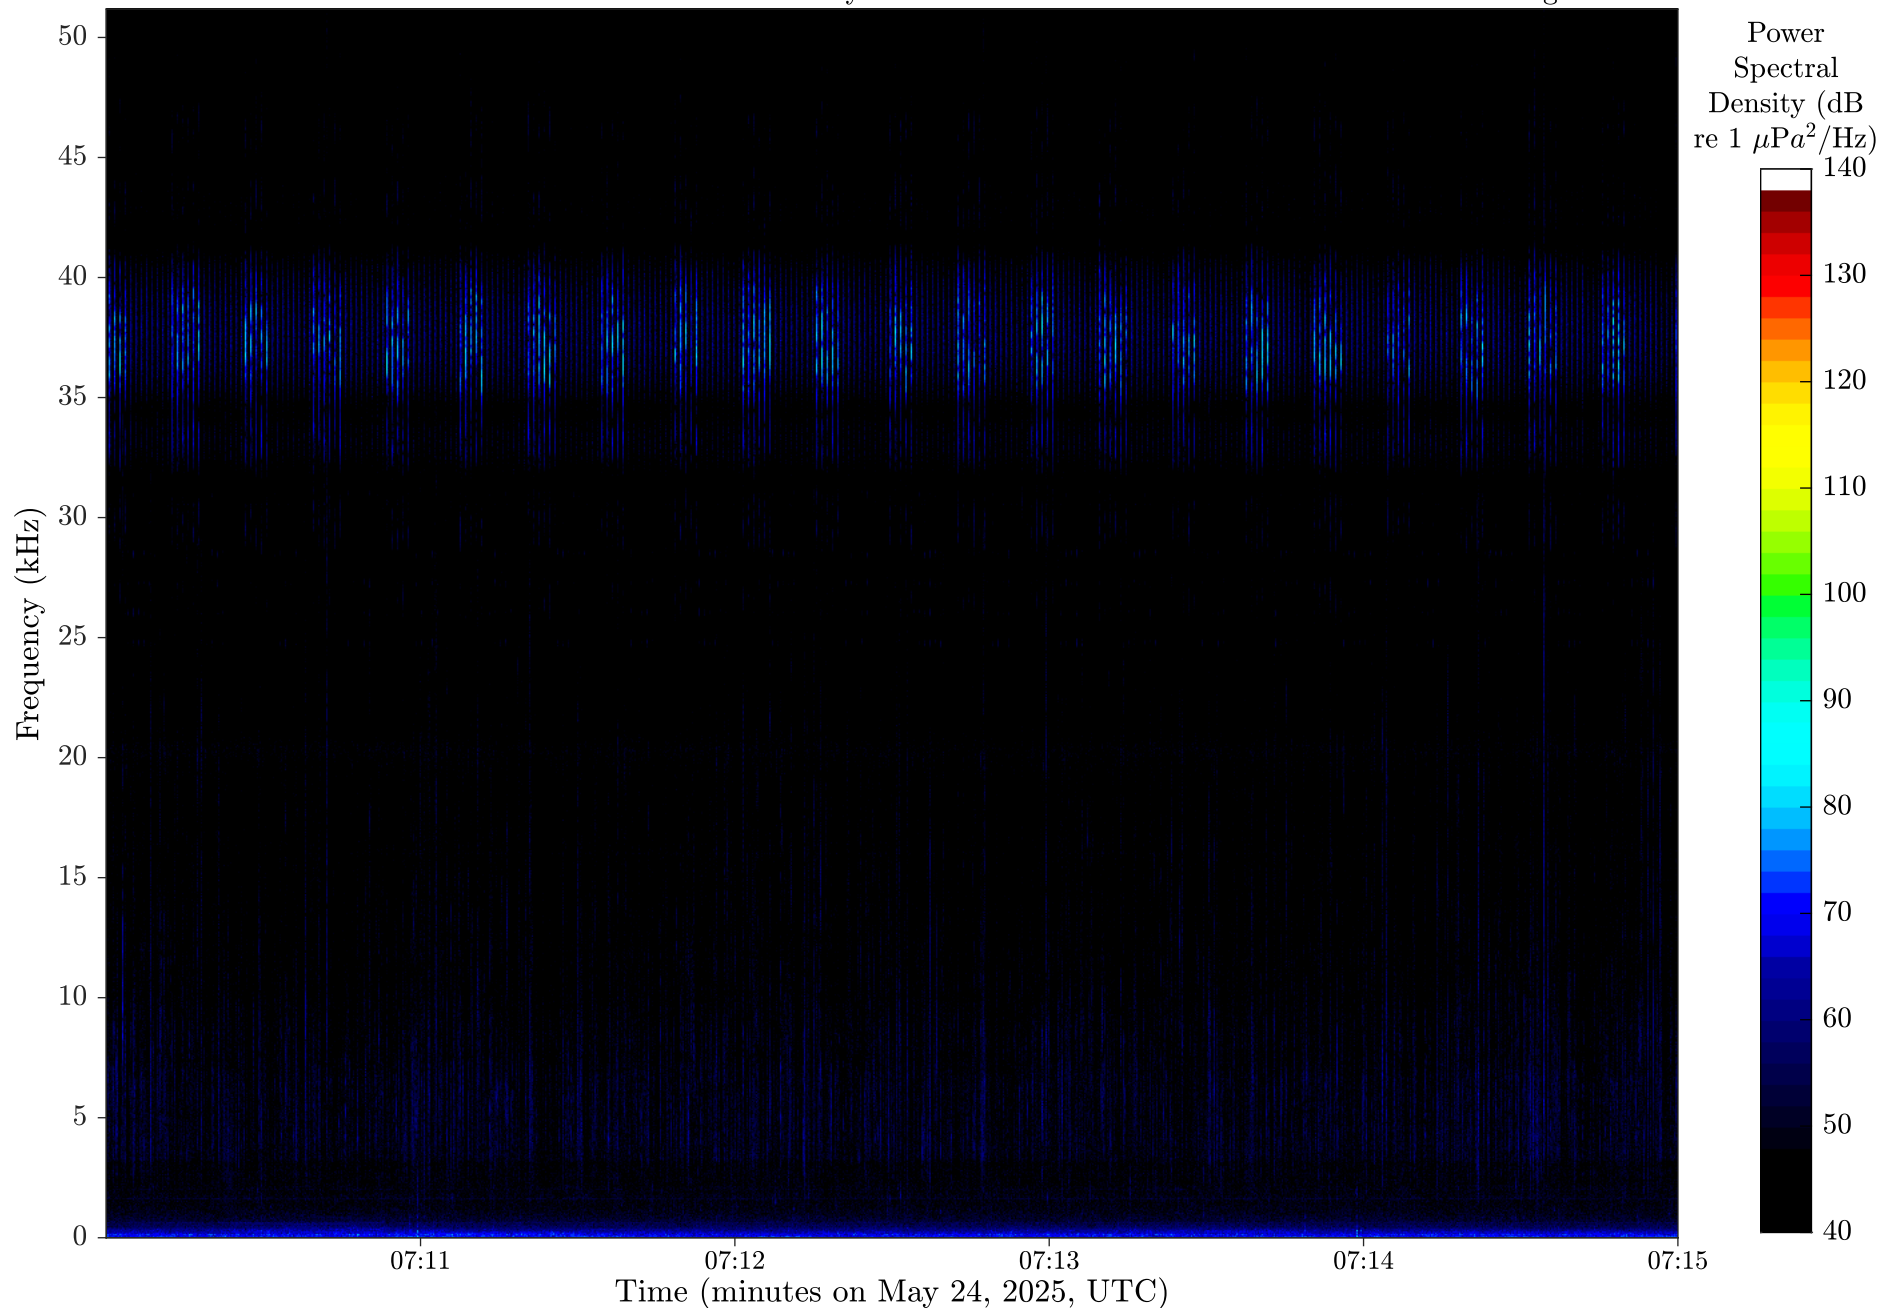



Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:26:53 UTC

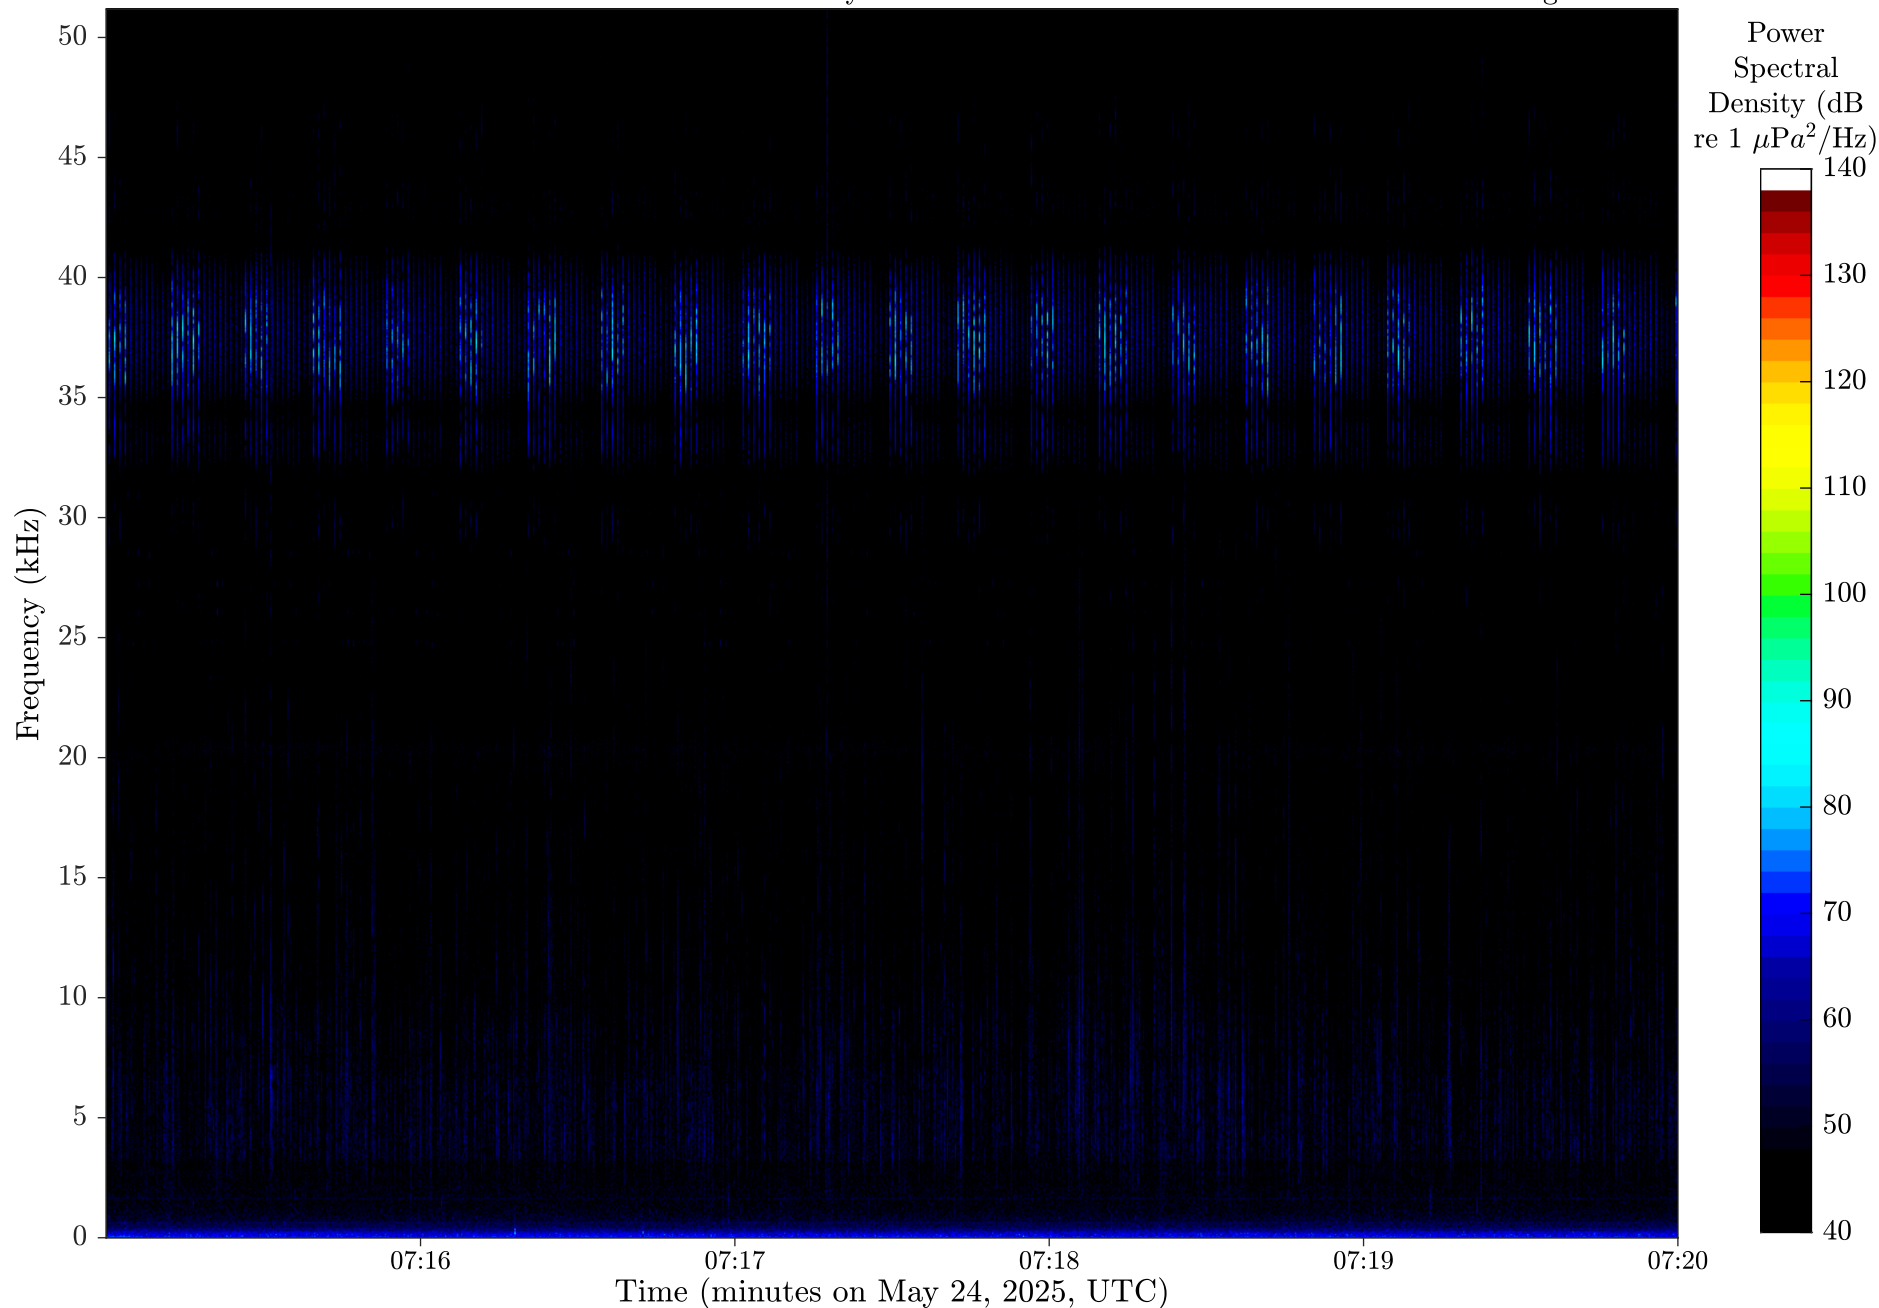

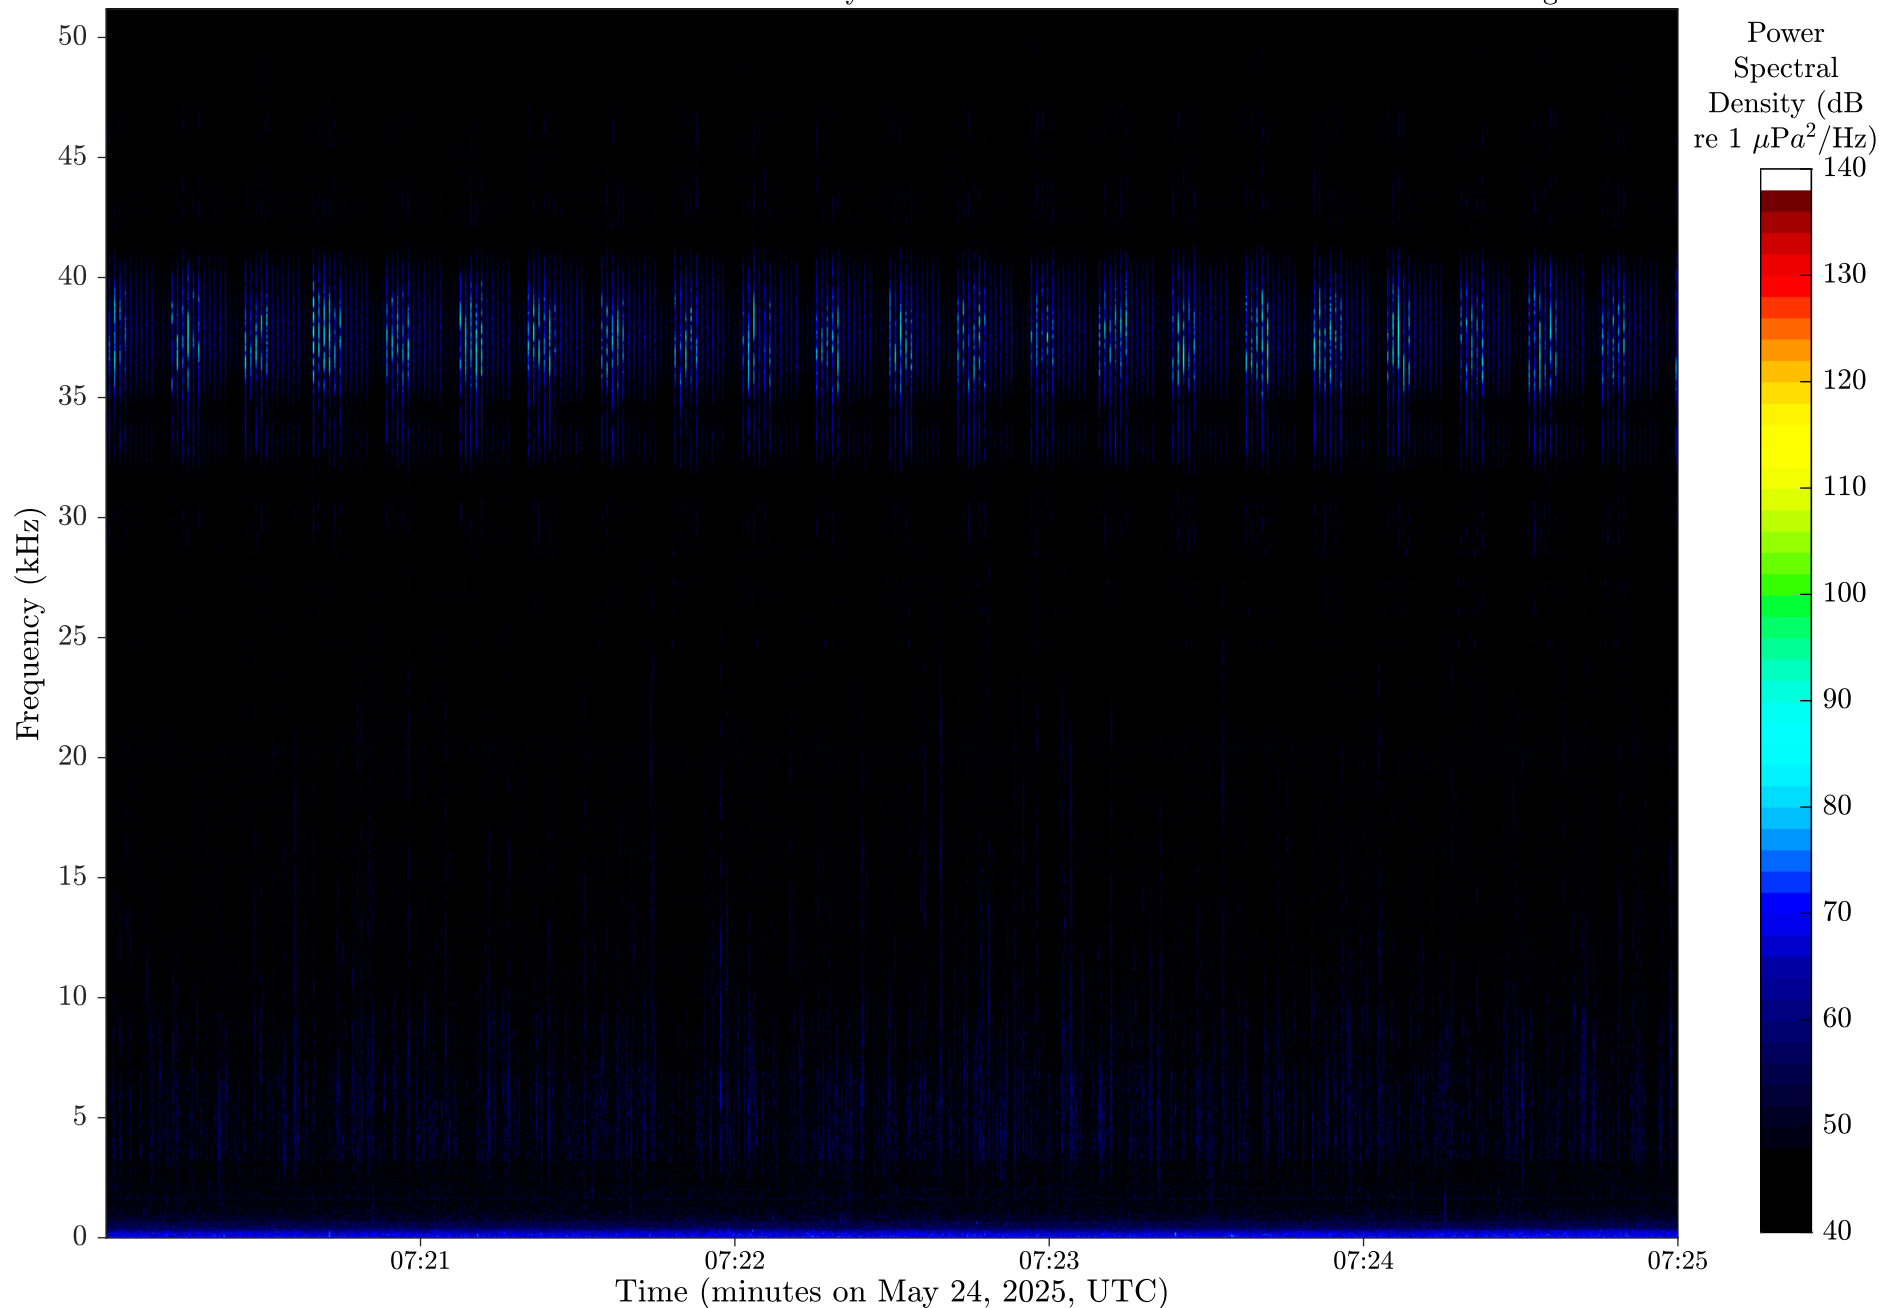


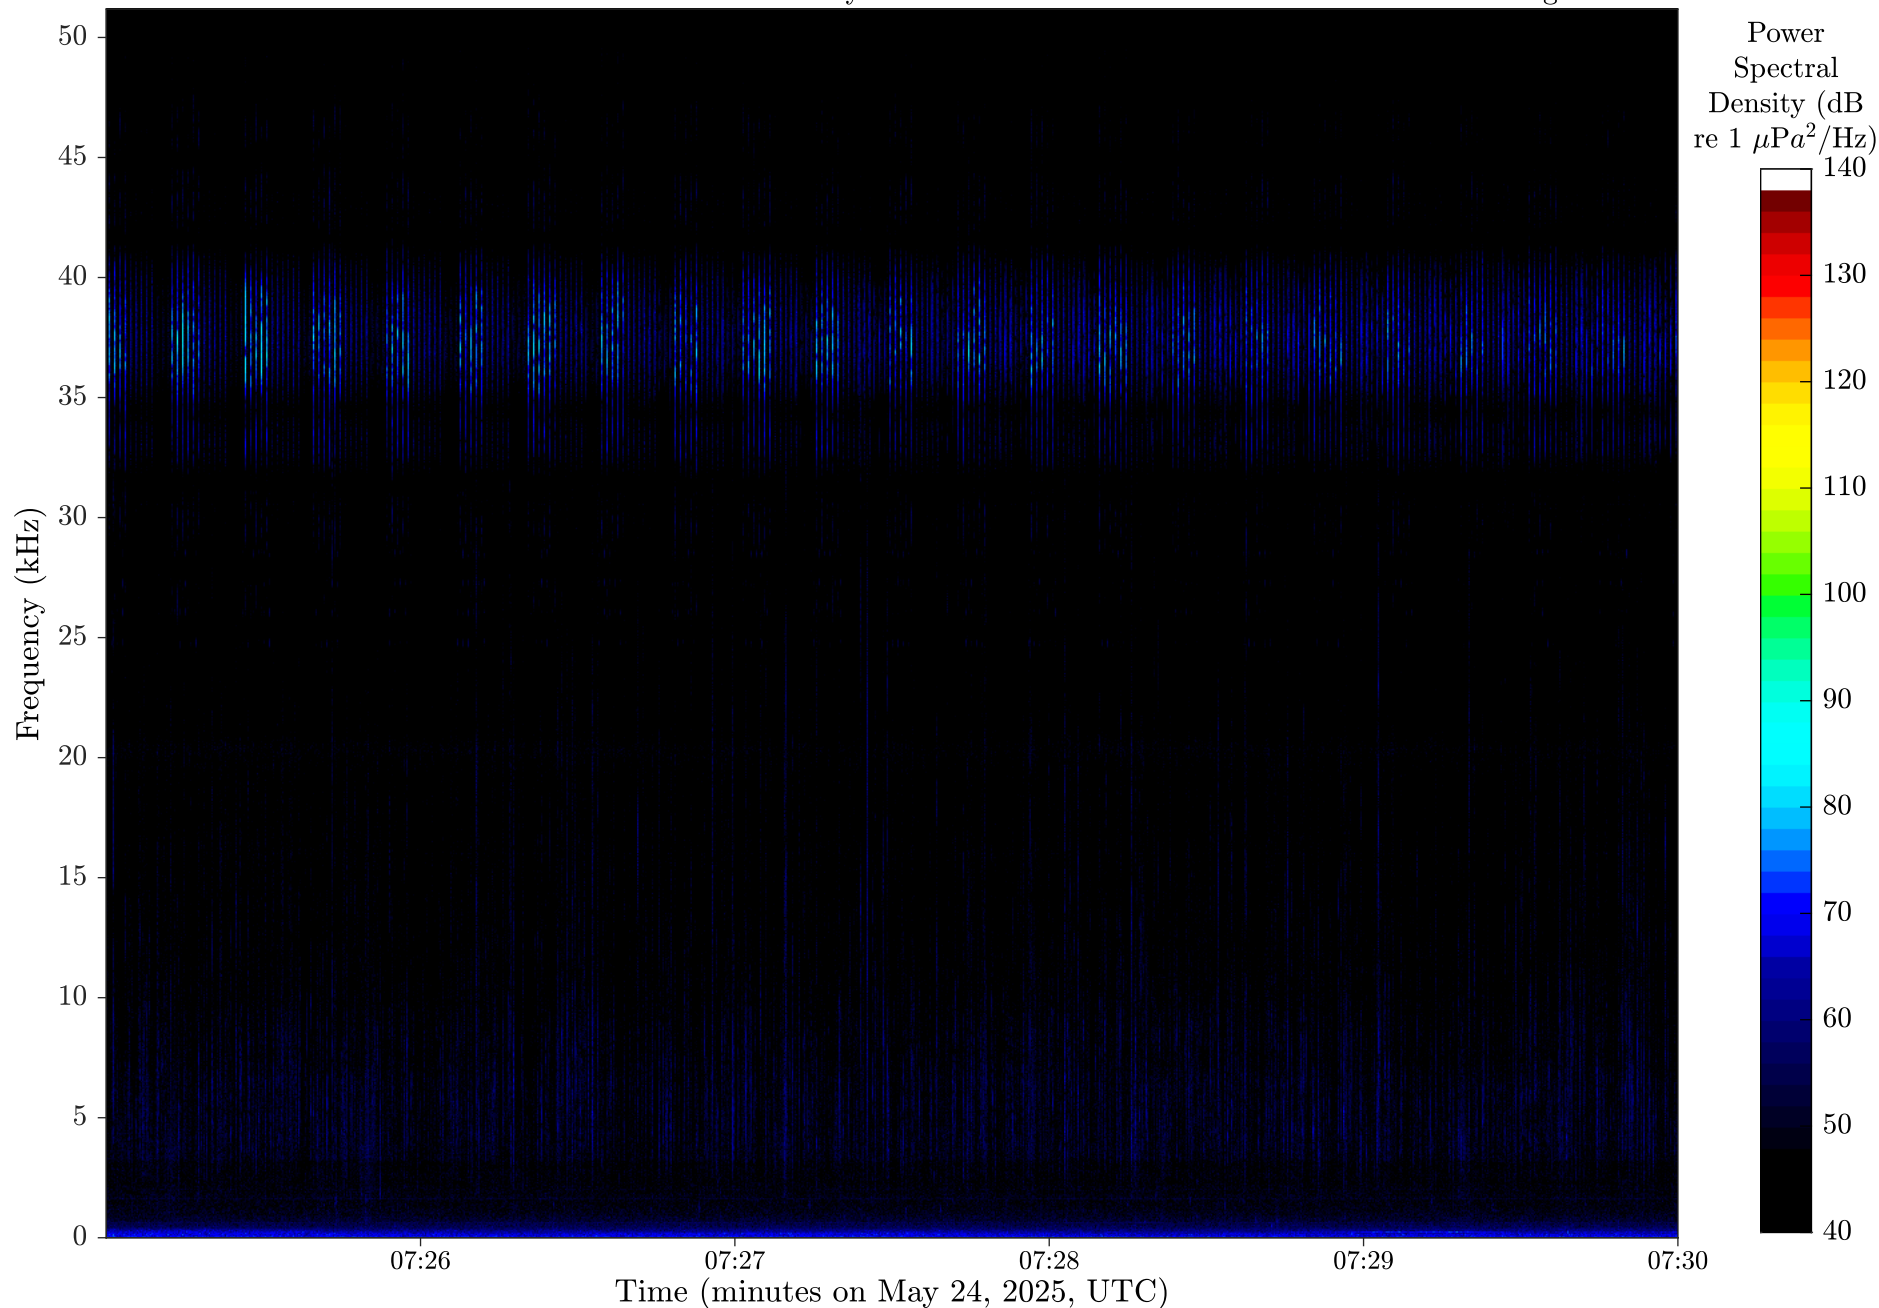


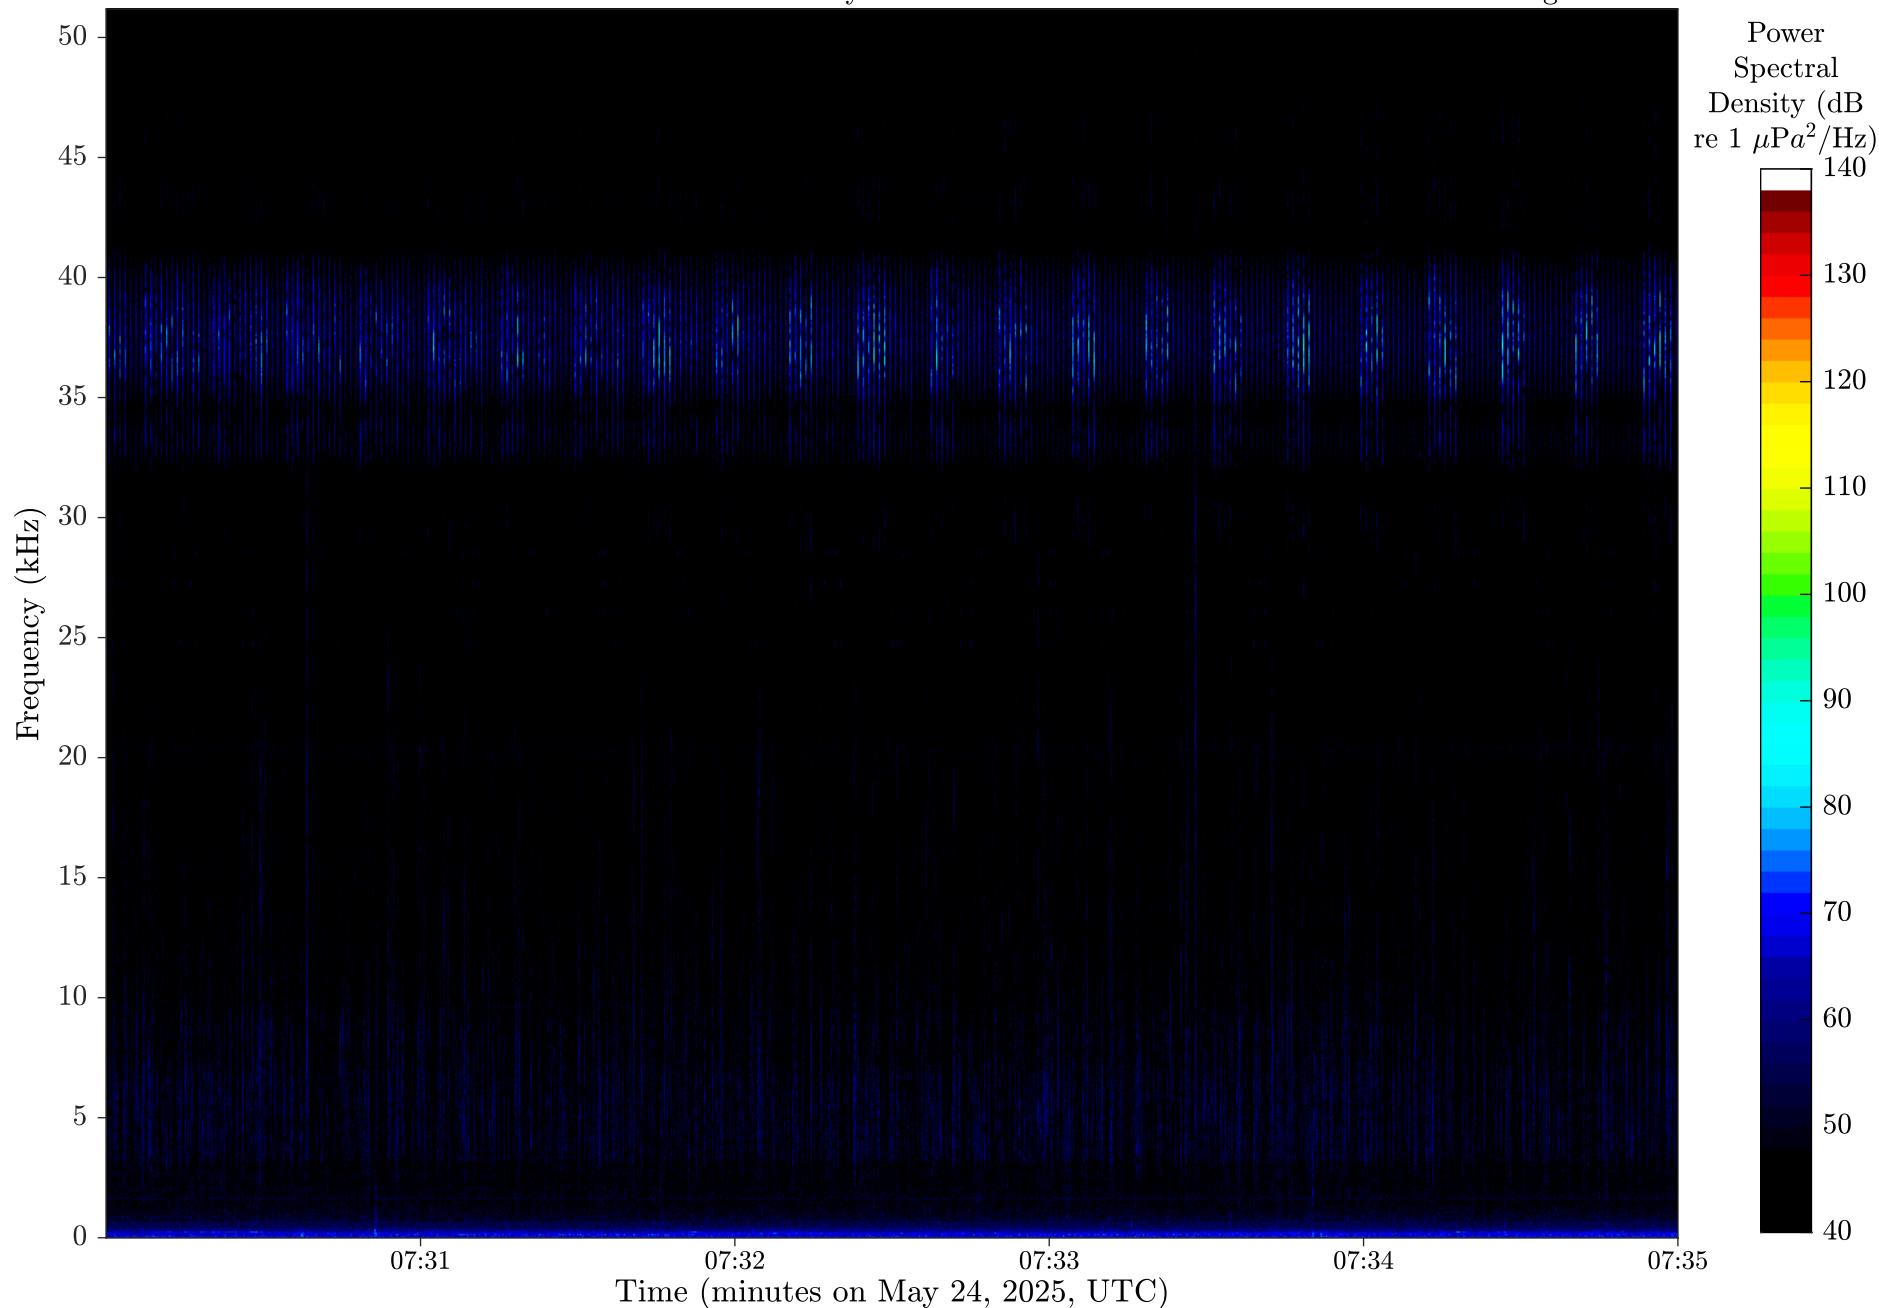

Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:27:30 UTC

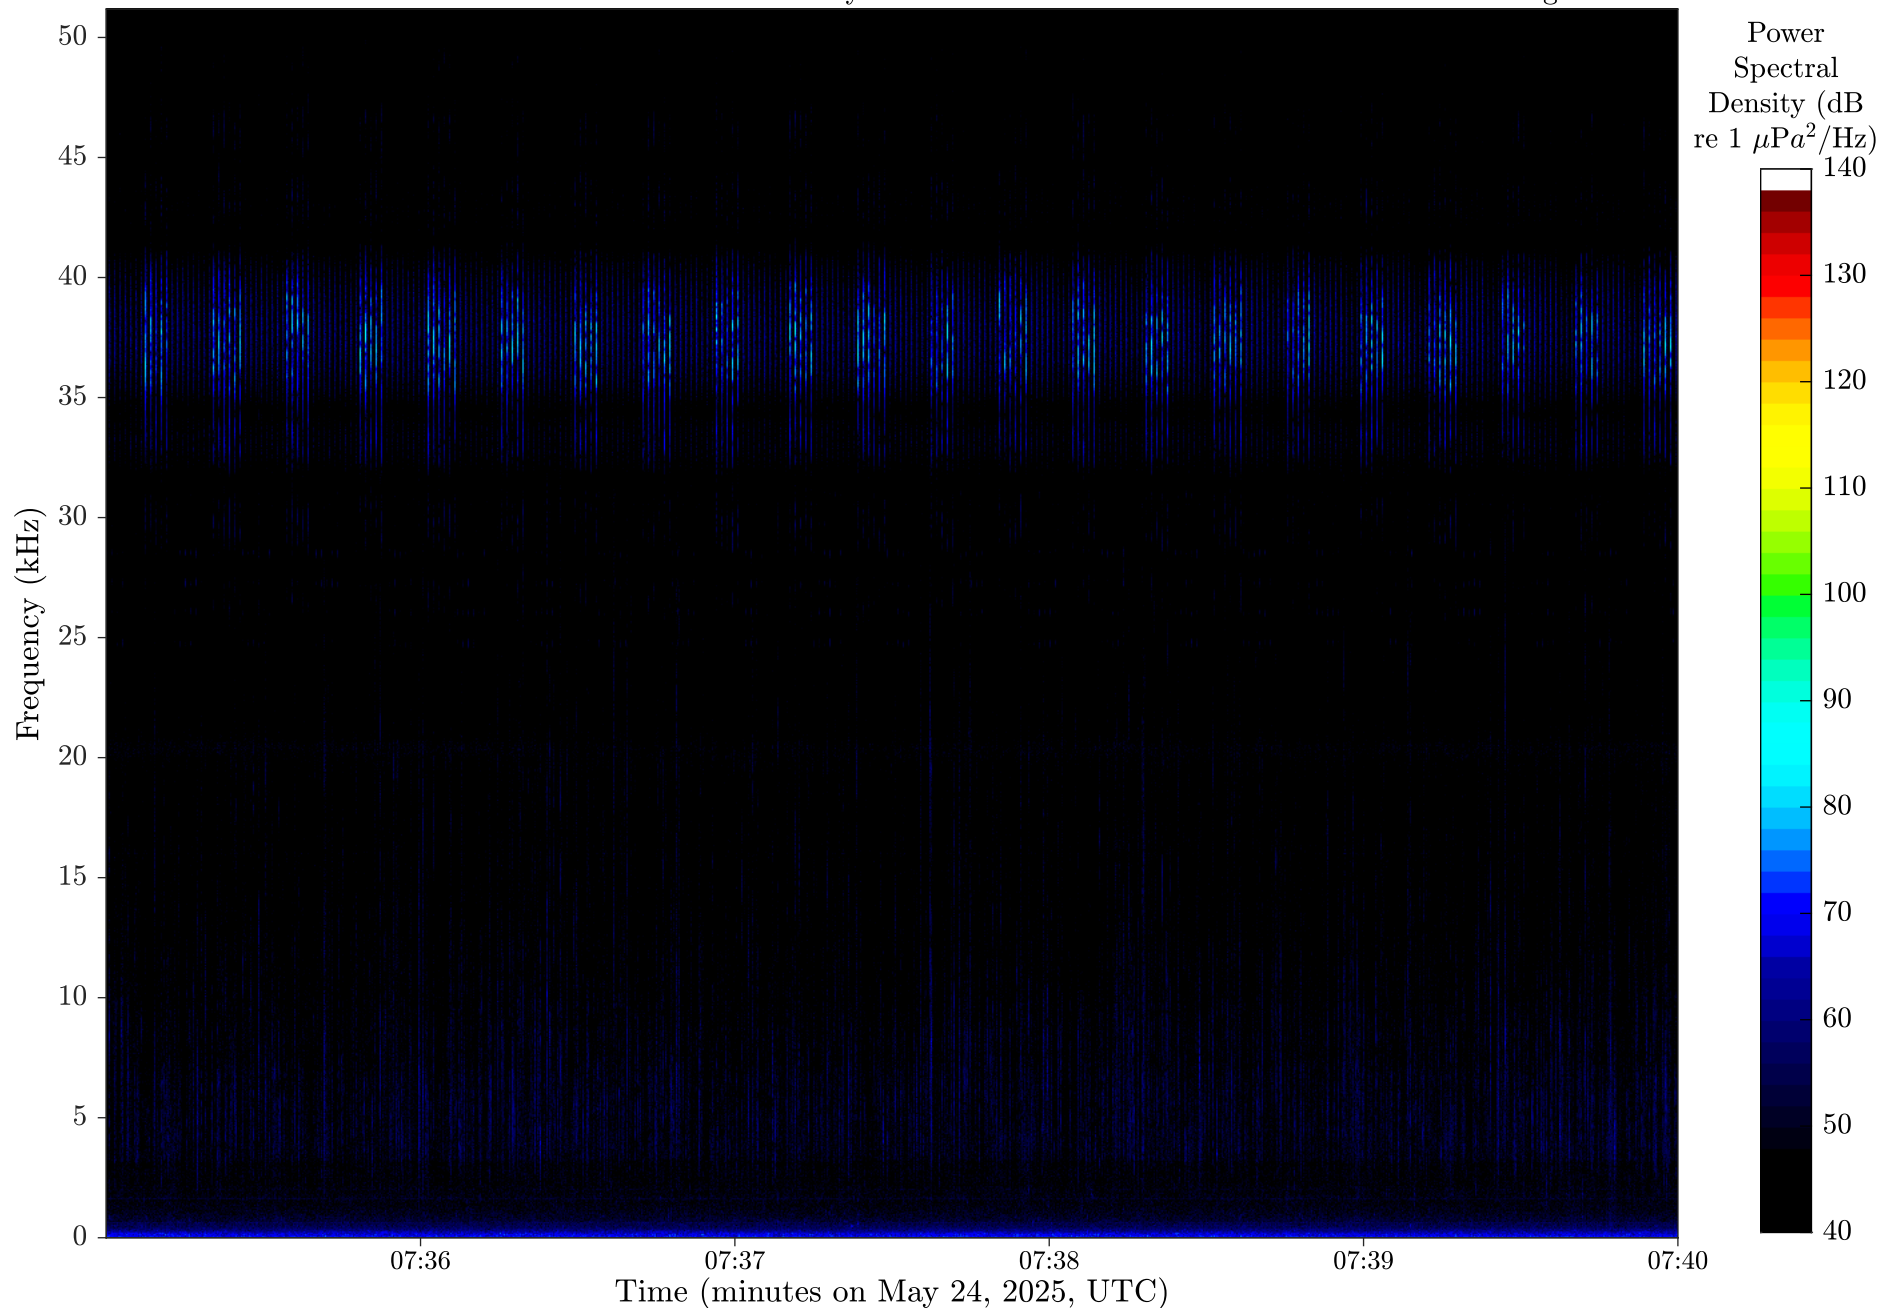

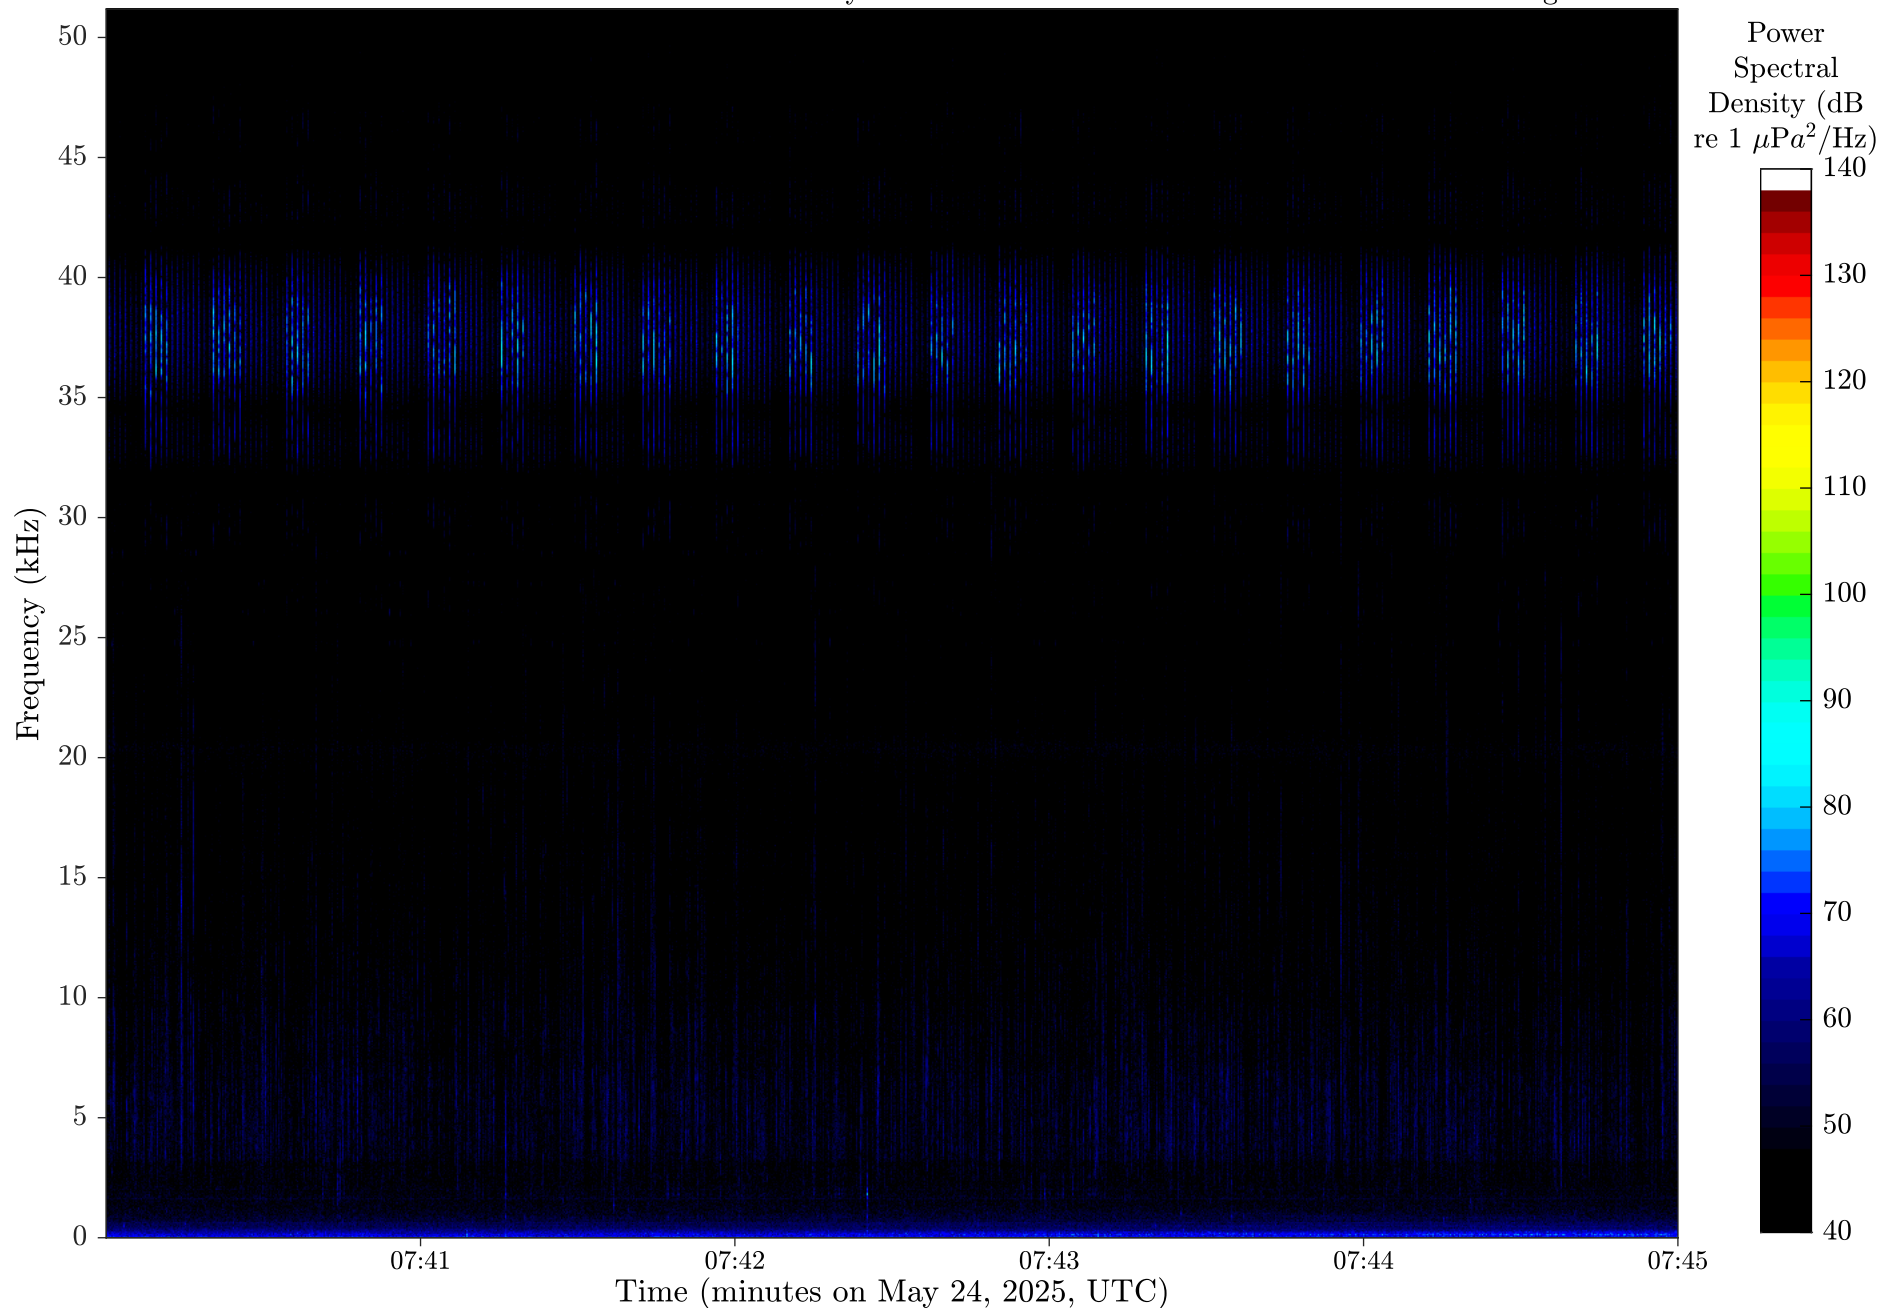


Comments: 36.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:27:48 UTC

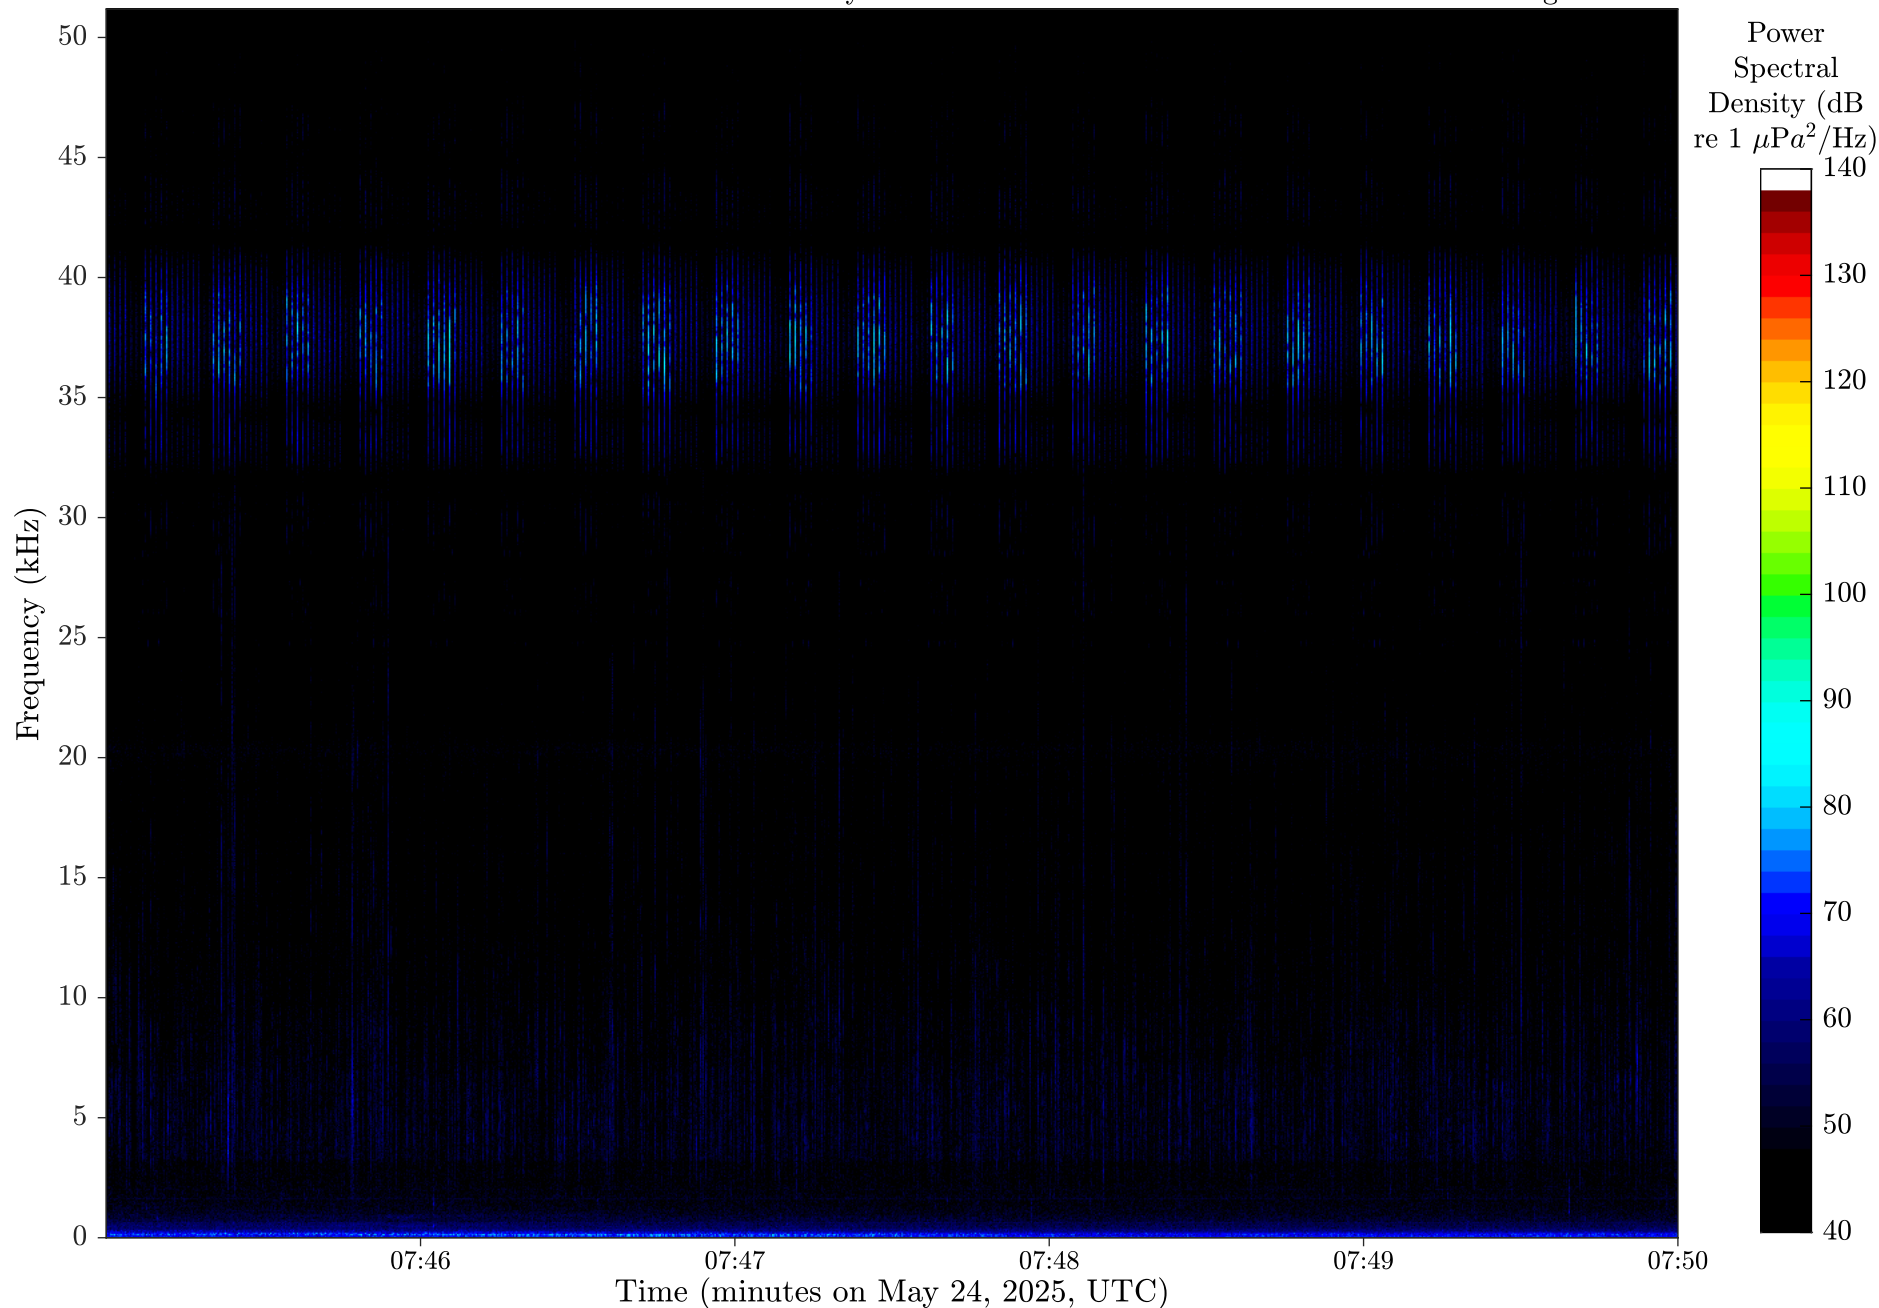


Comments: 36.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:27:57 UTC

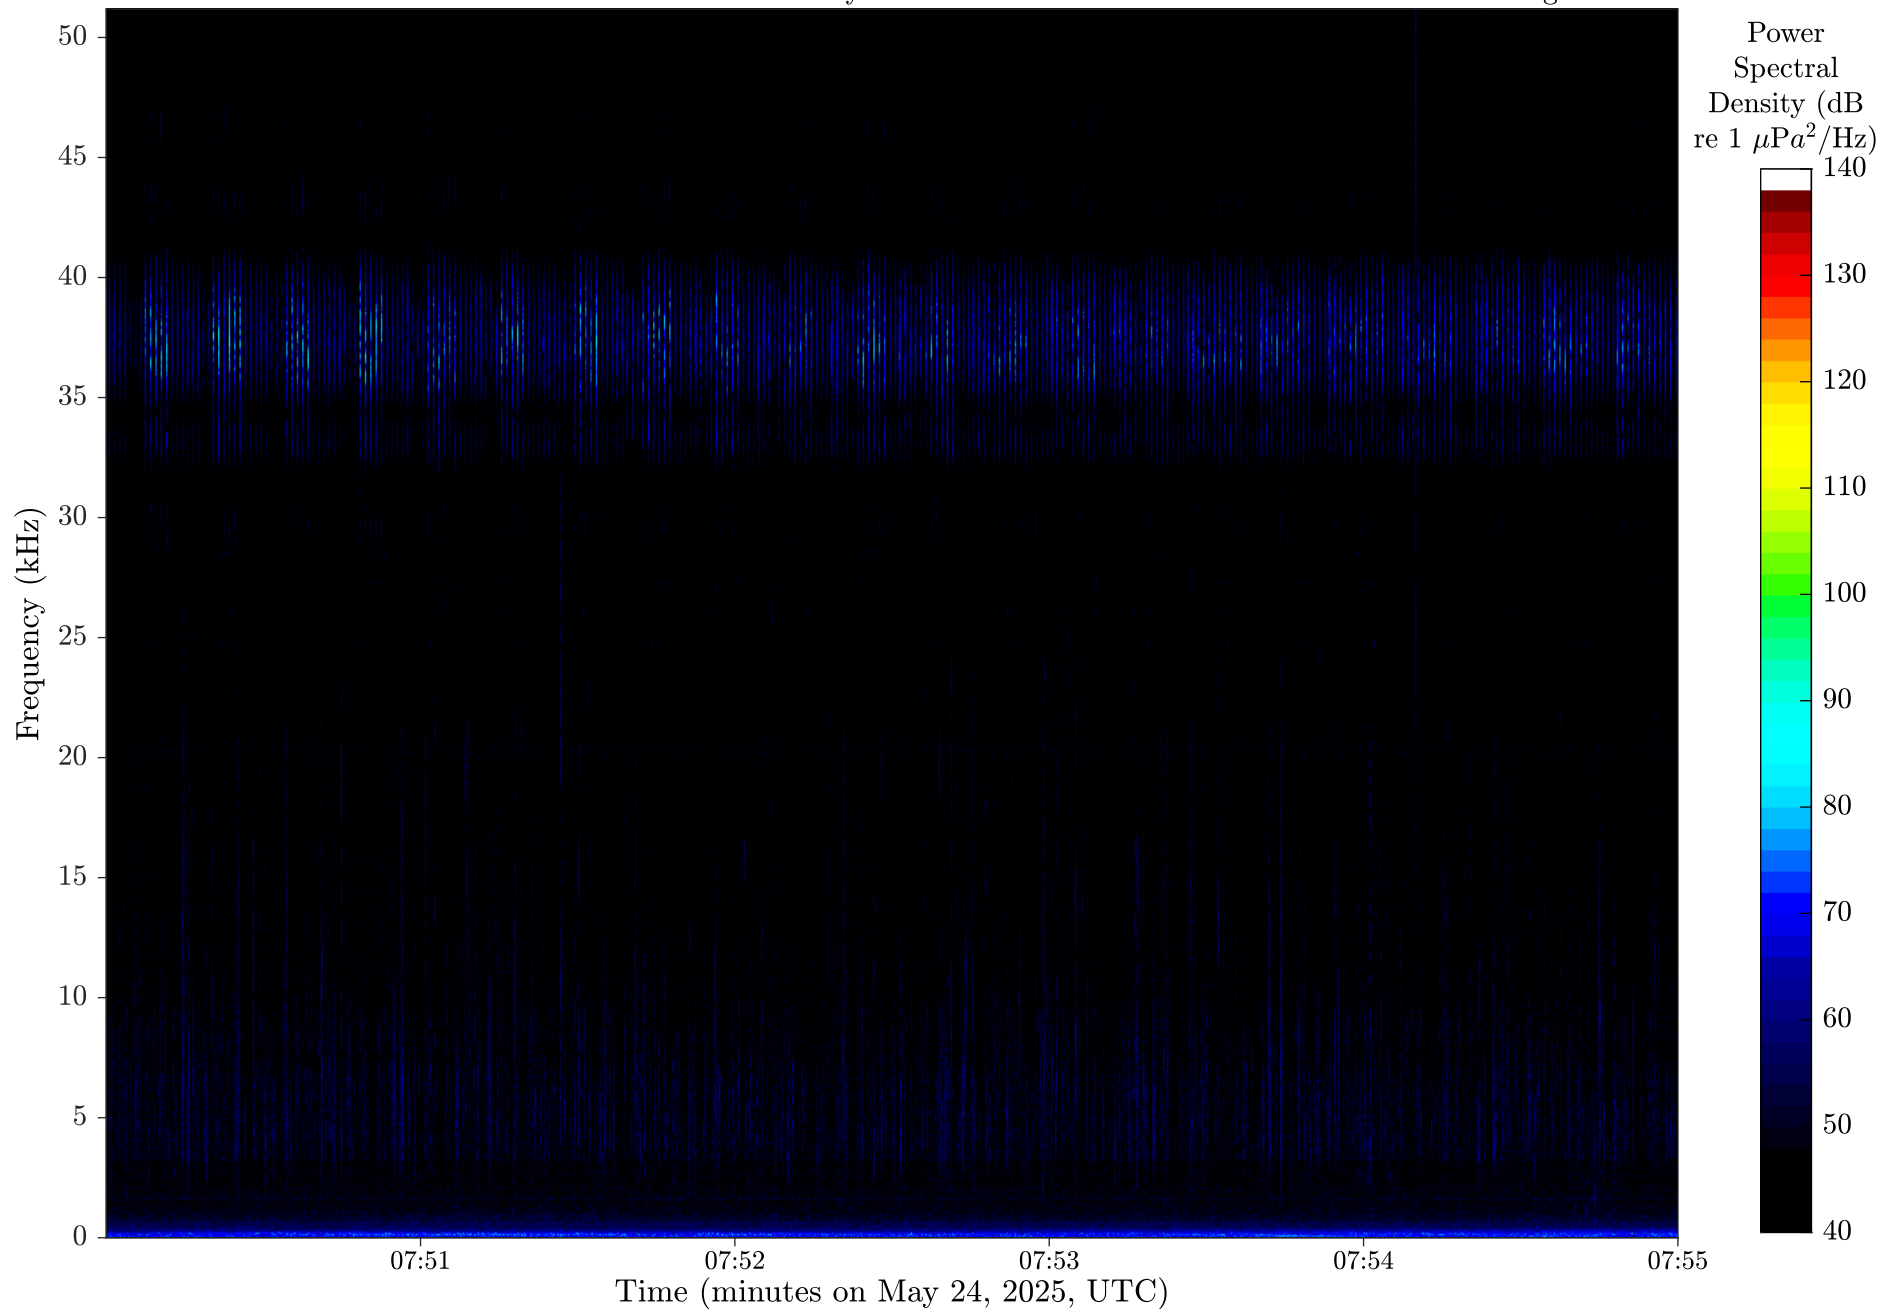


Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:28:06 UTC

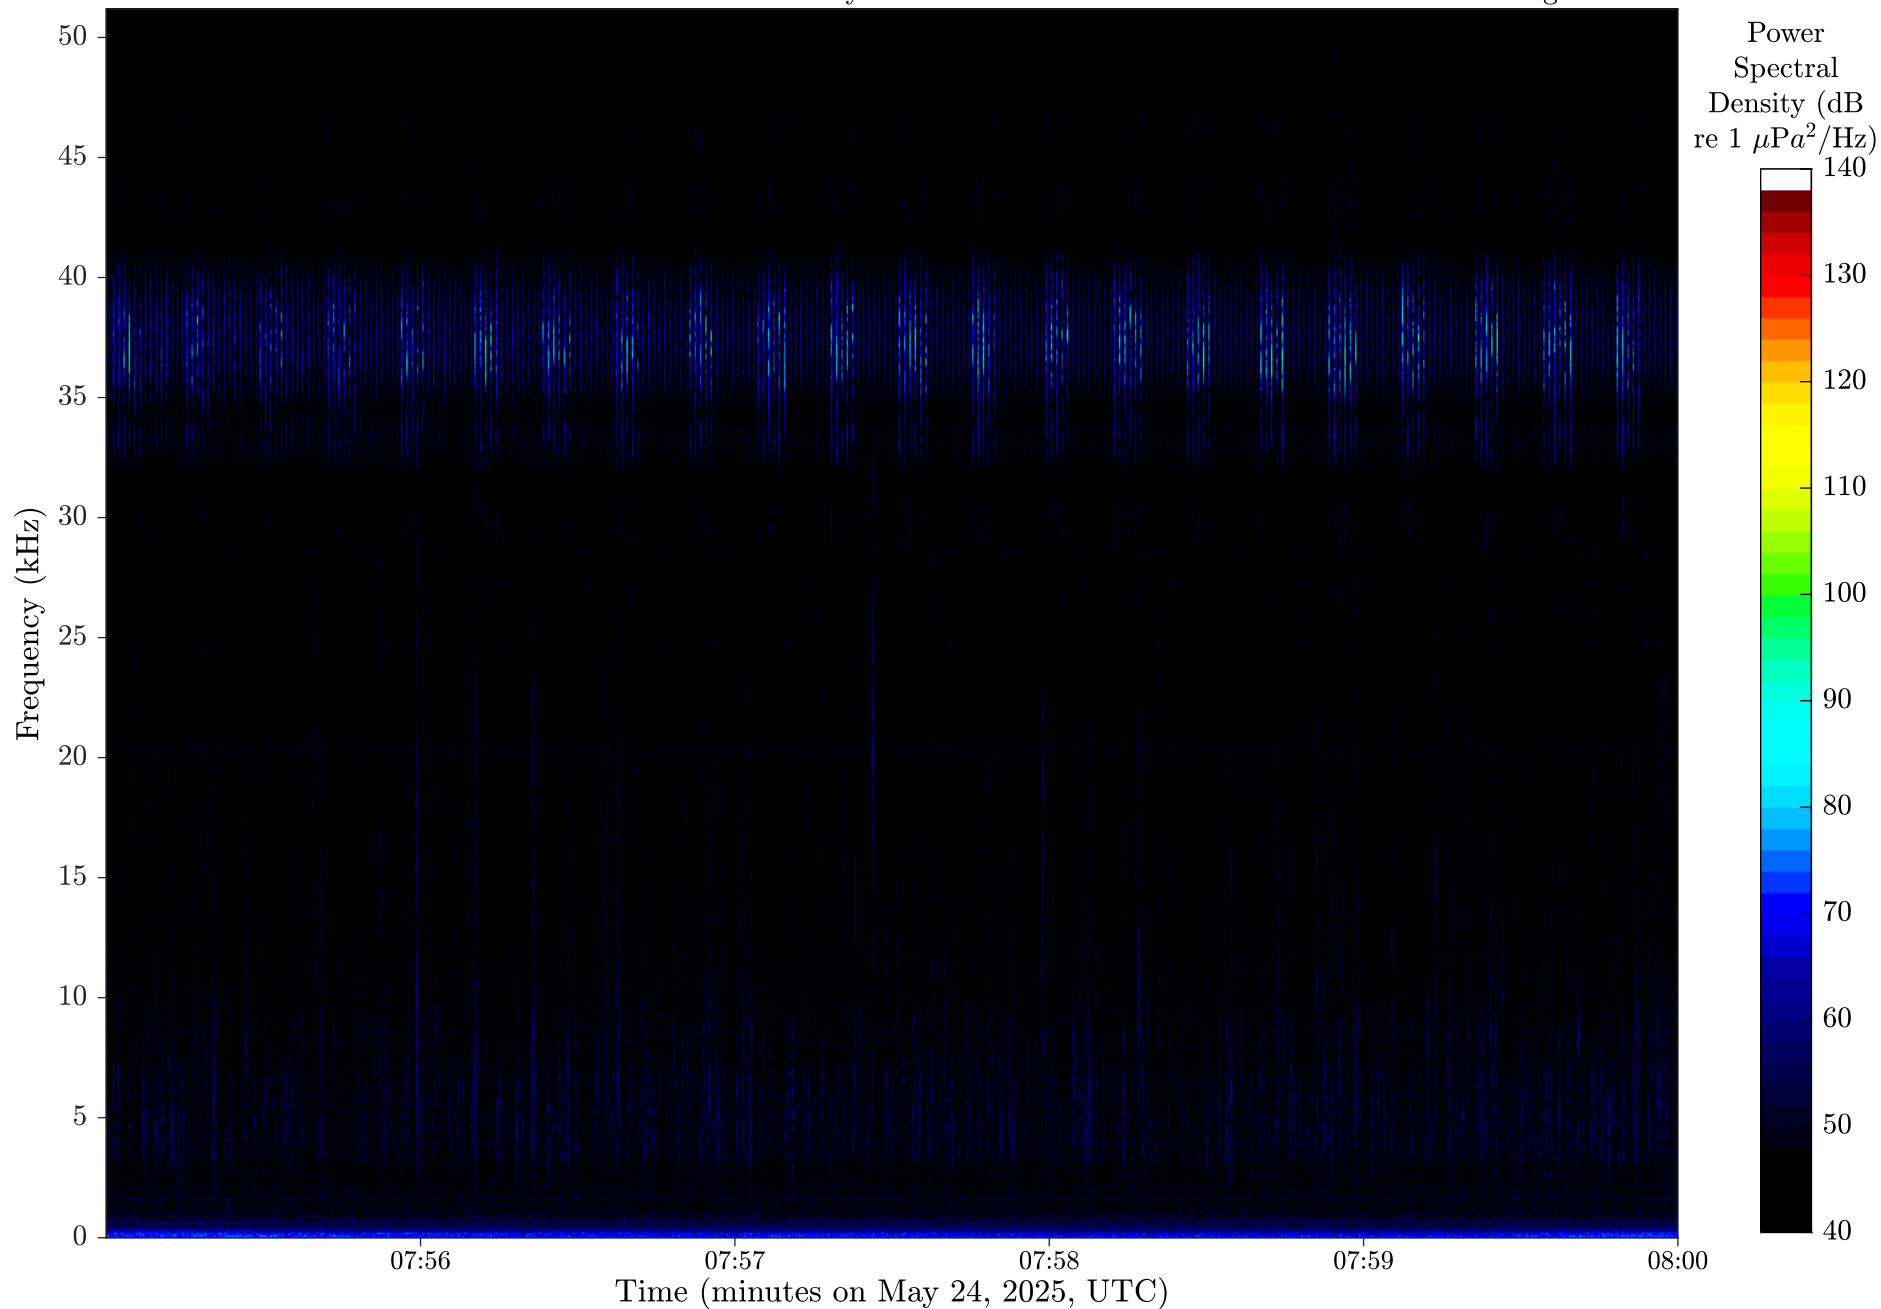

Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:28:14 UTC

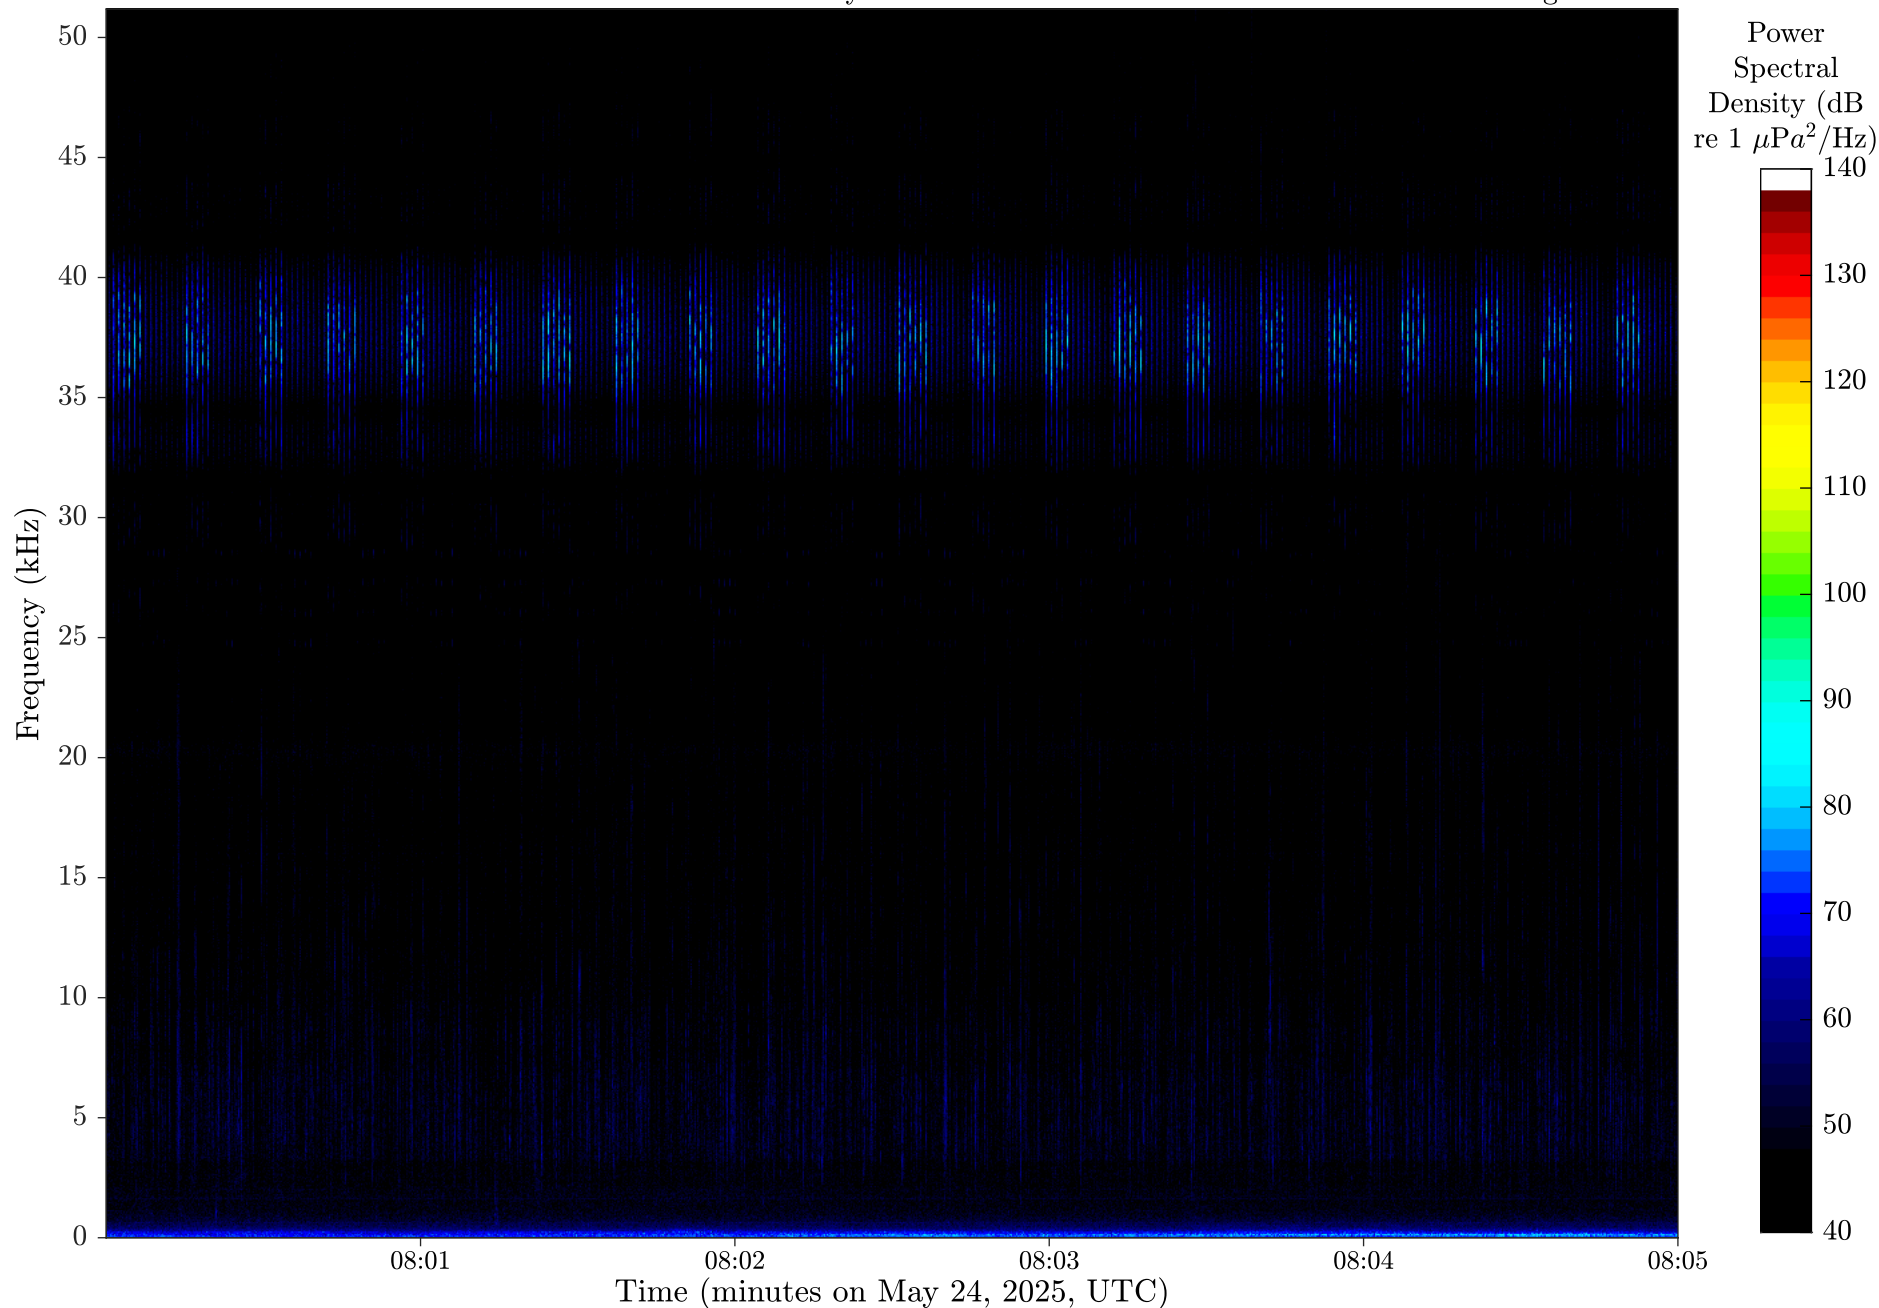

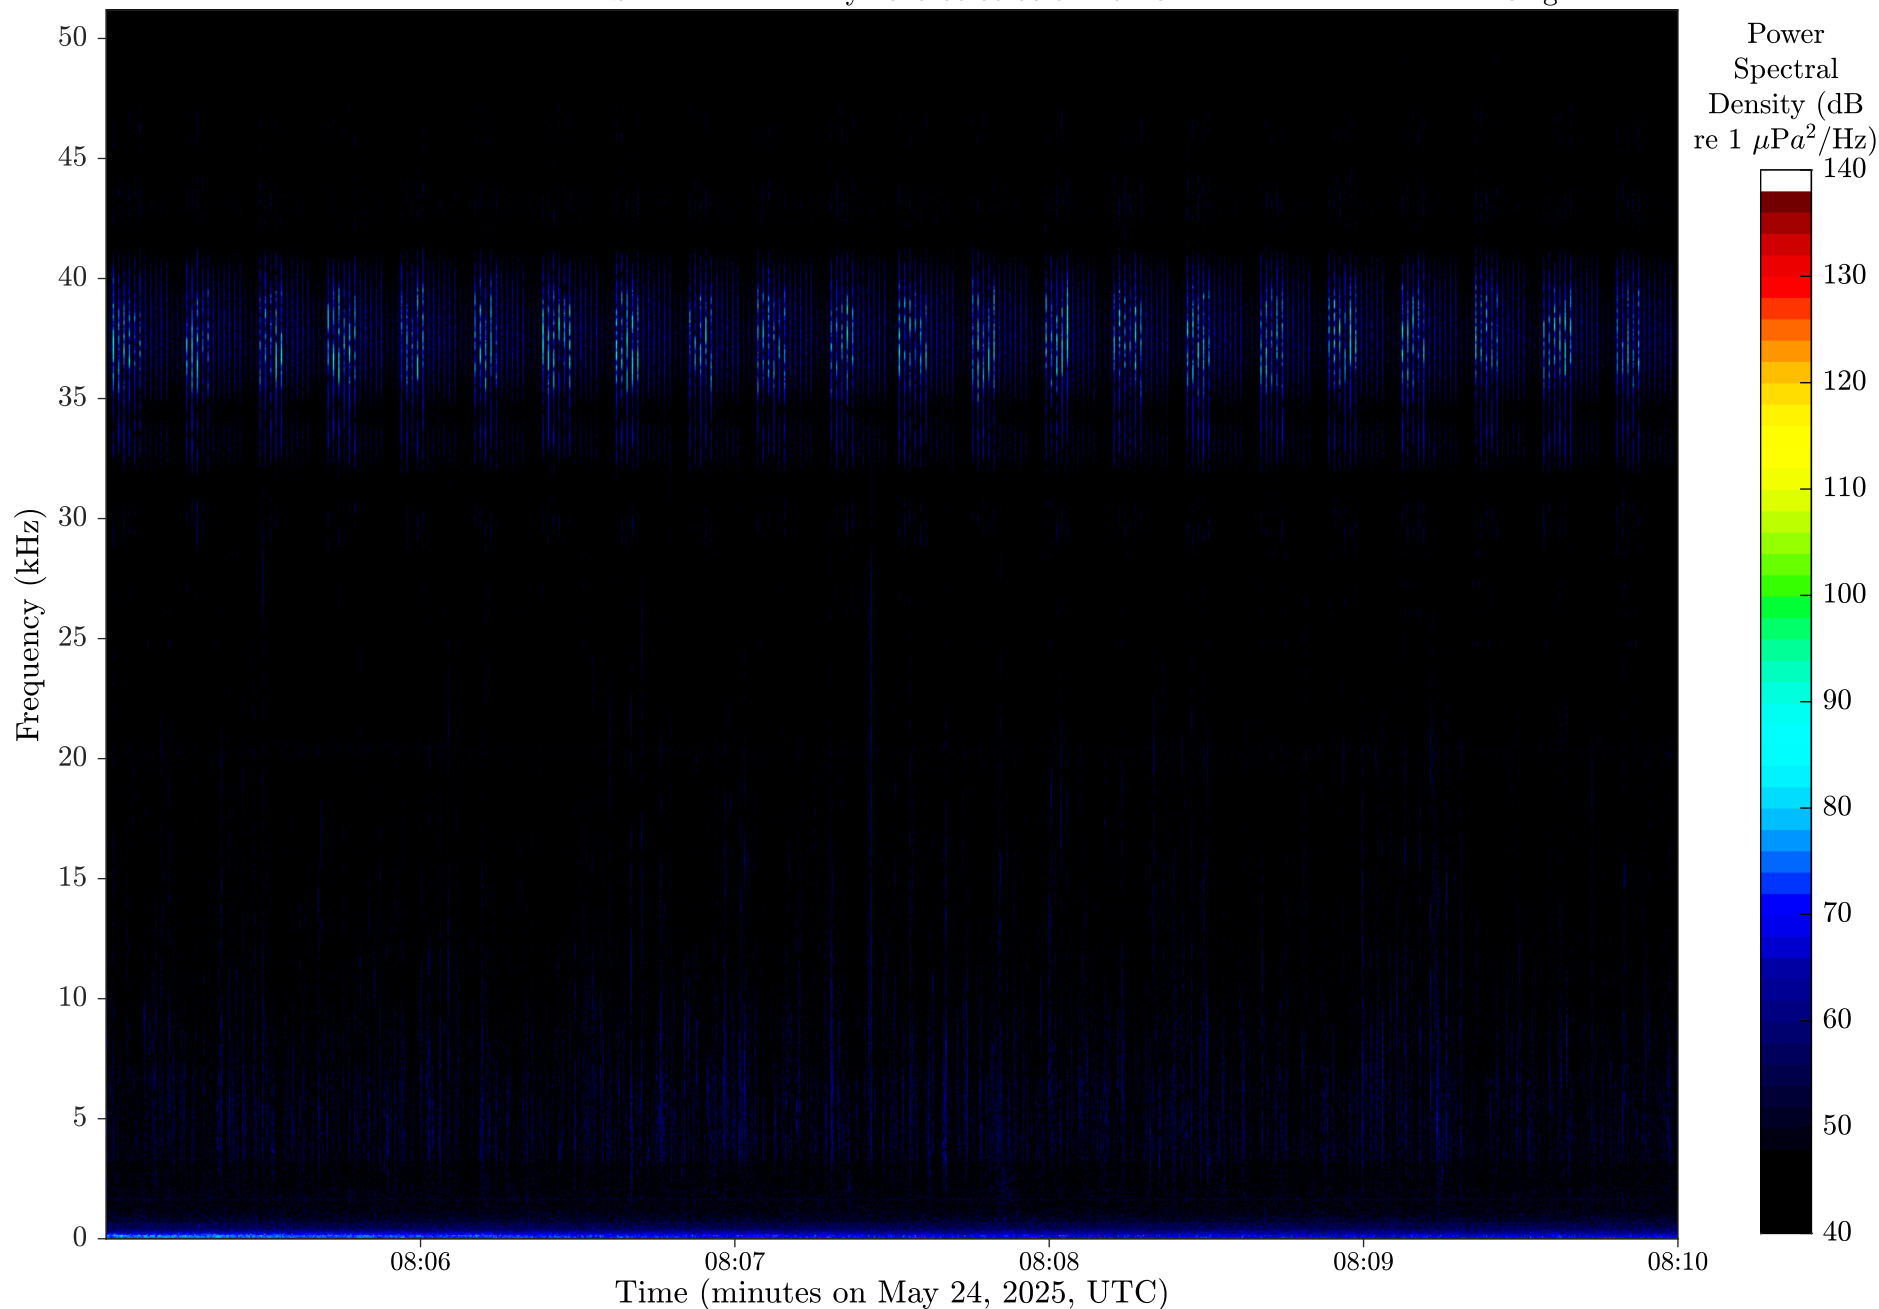


Comments: 36.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:28:30 UTC

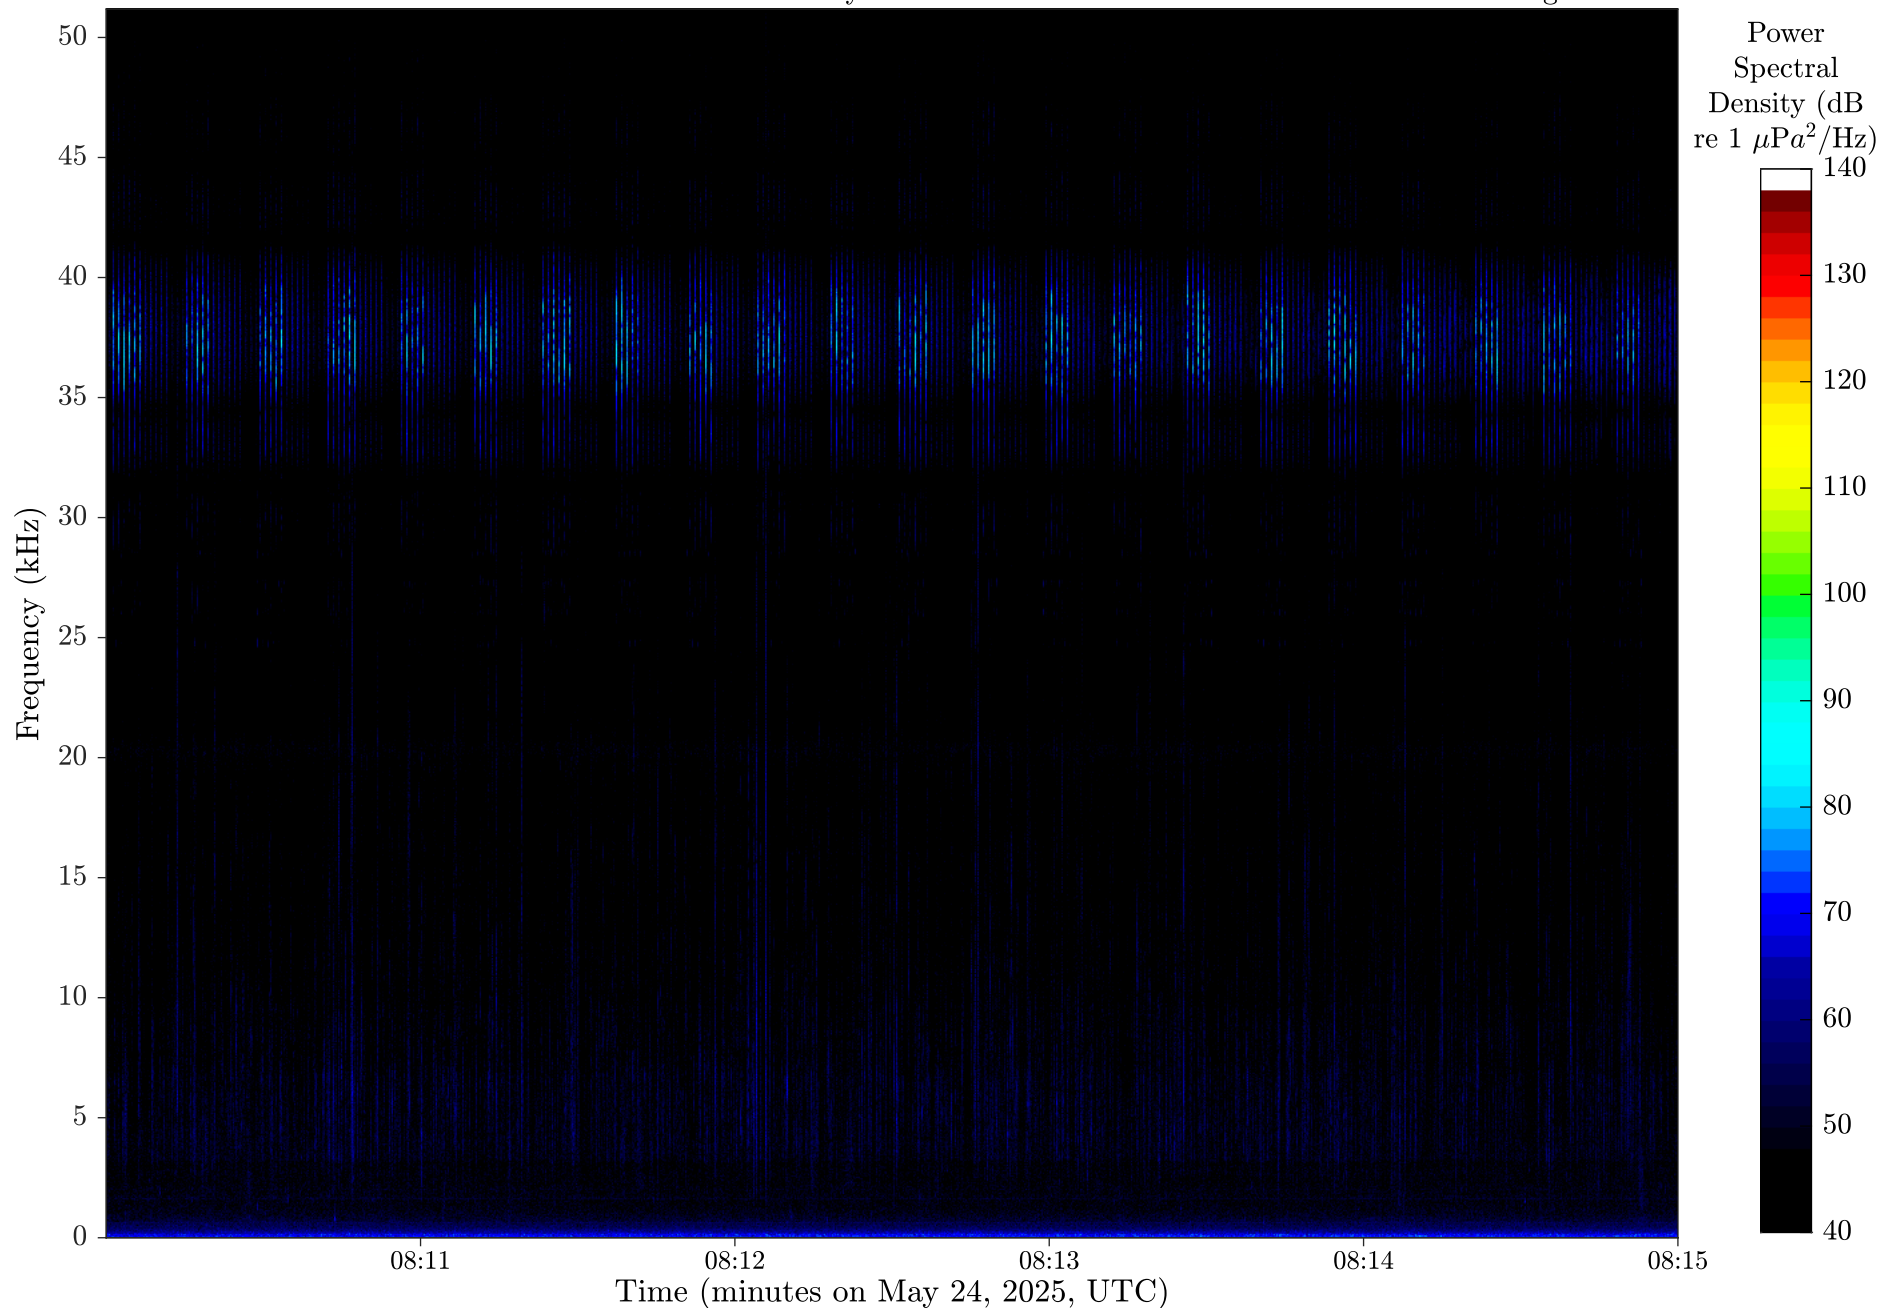

Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:28:39 UTC

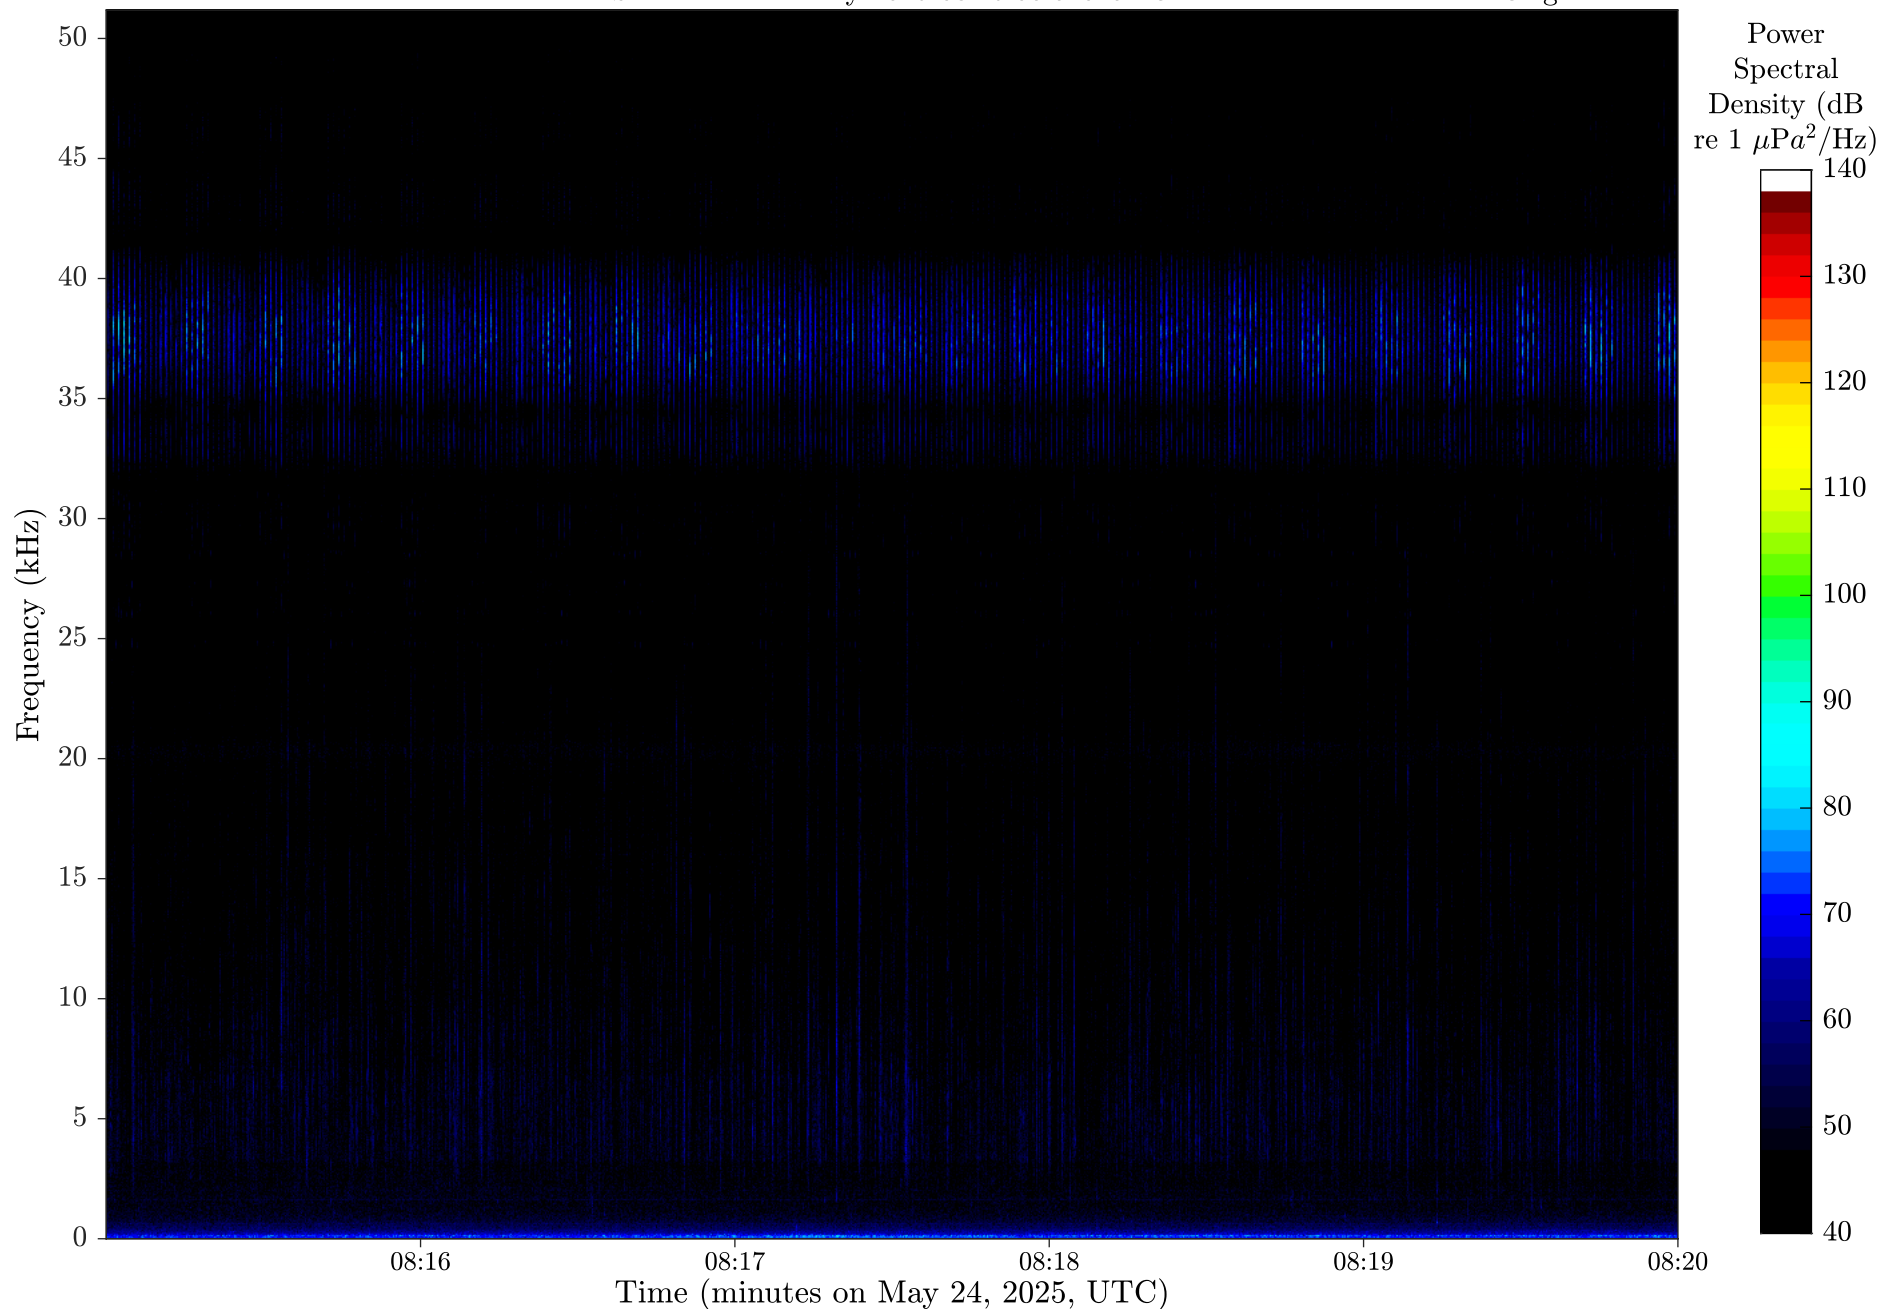

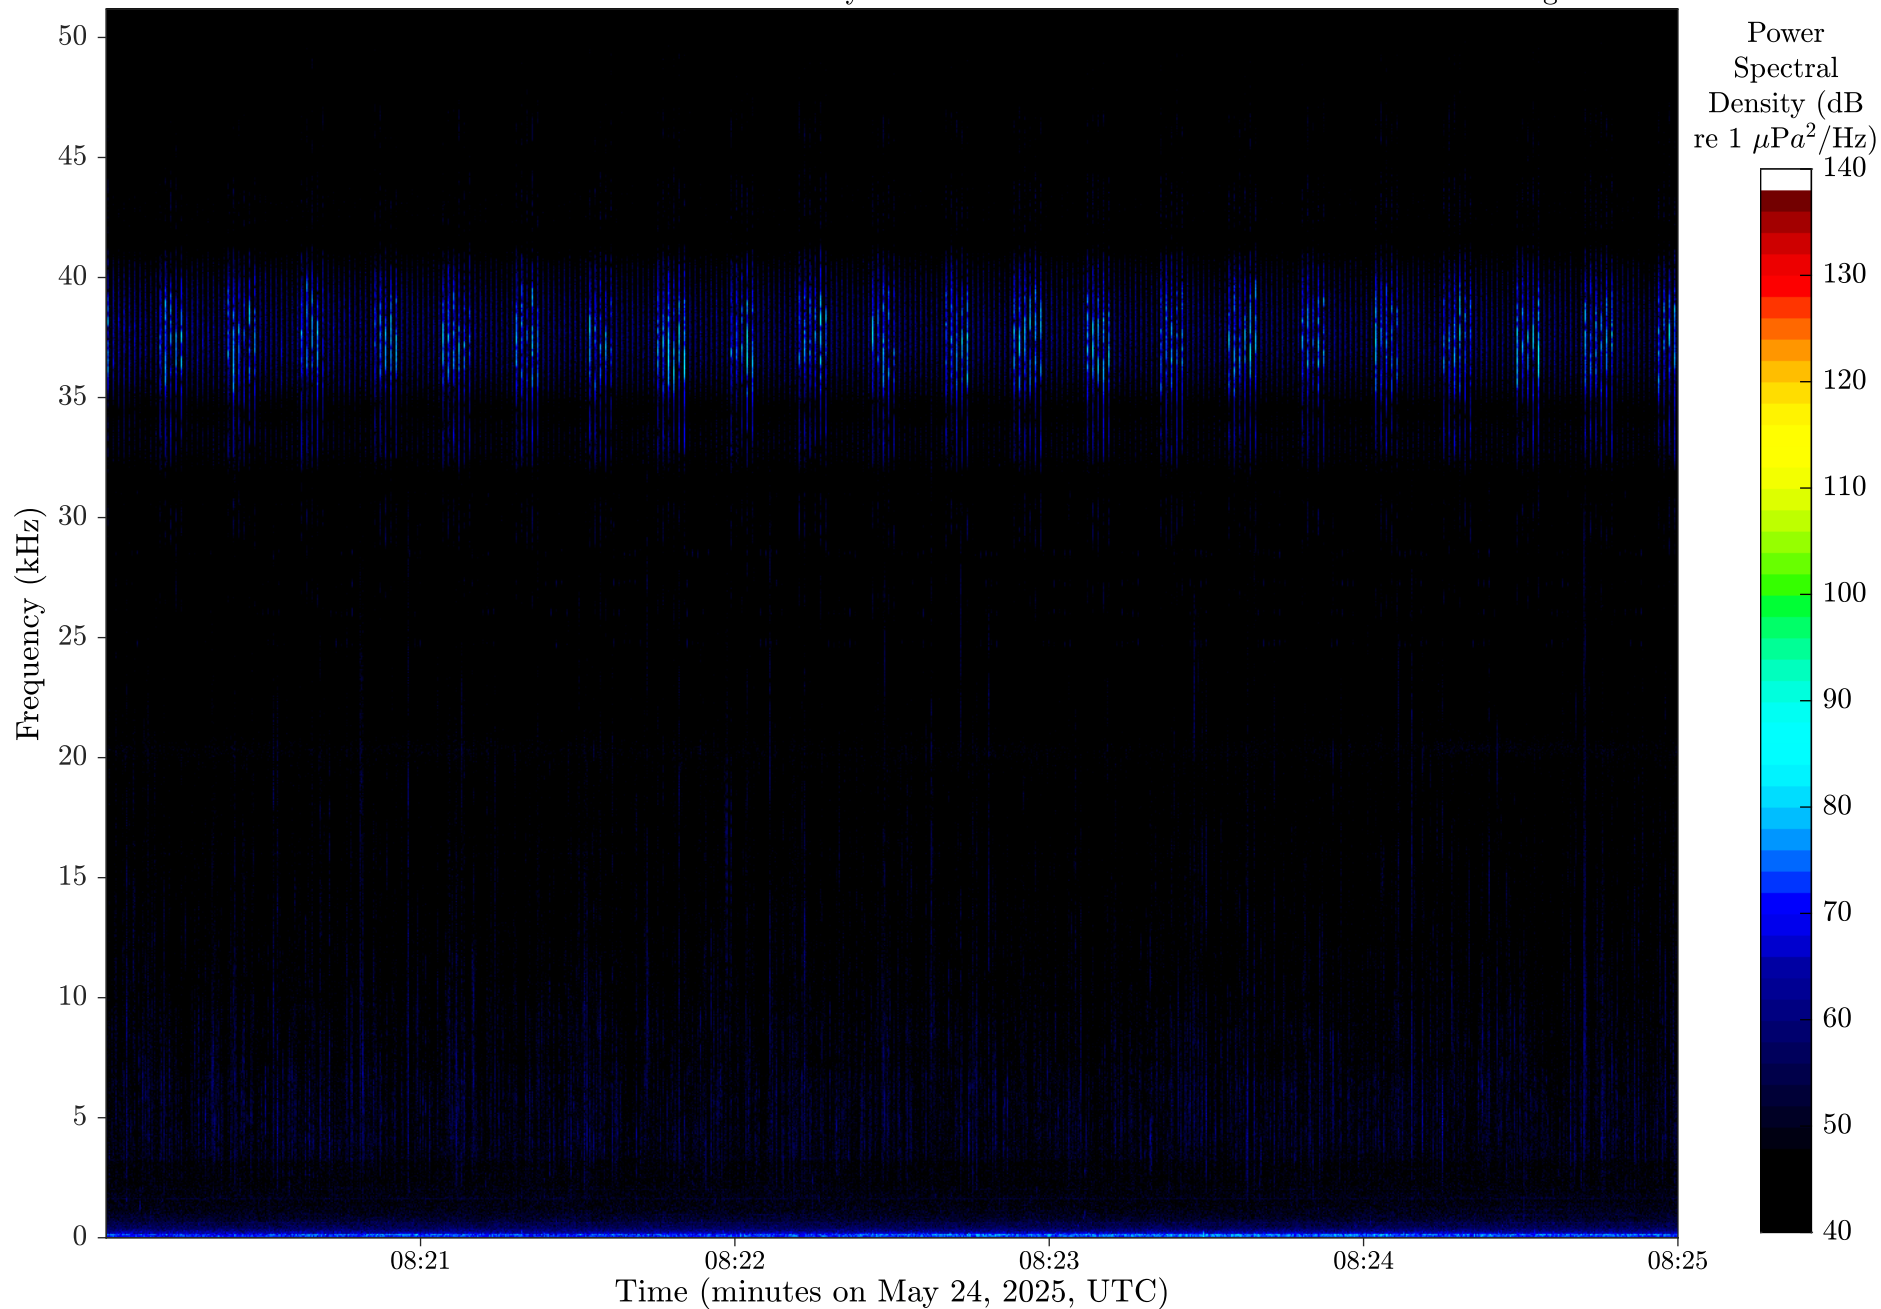


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:28:55 UTC

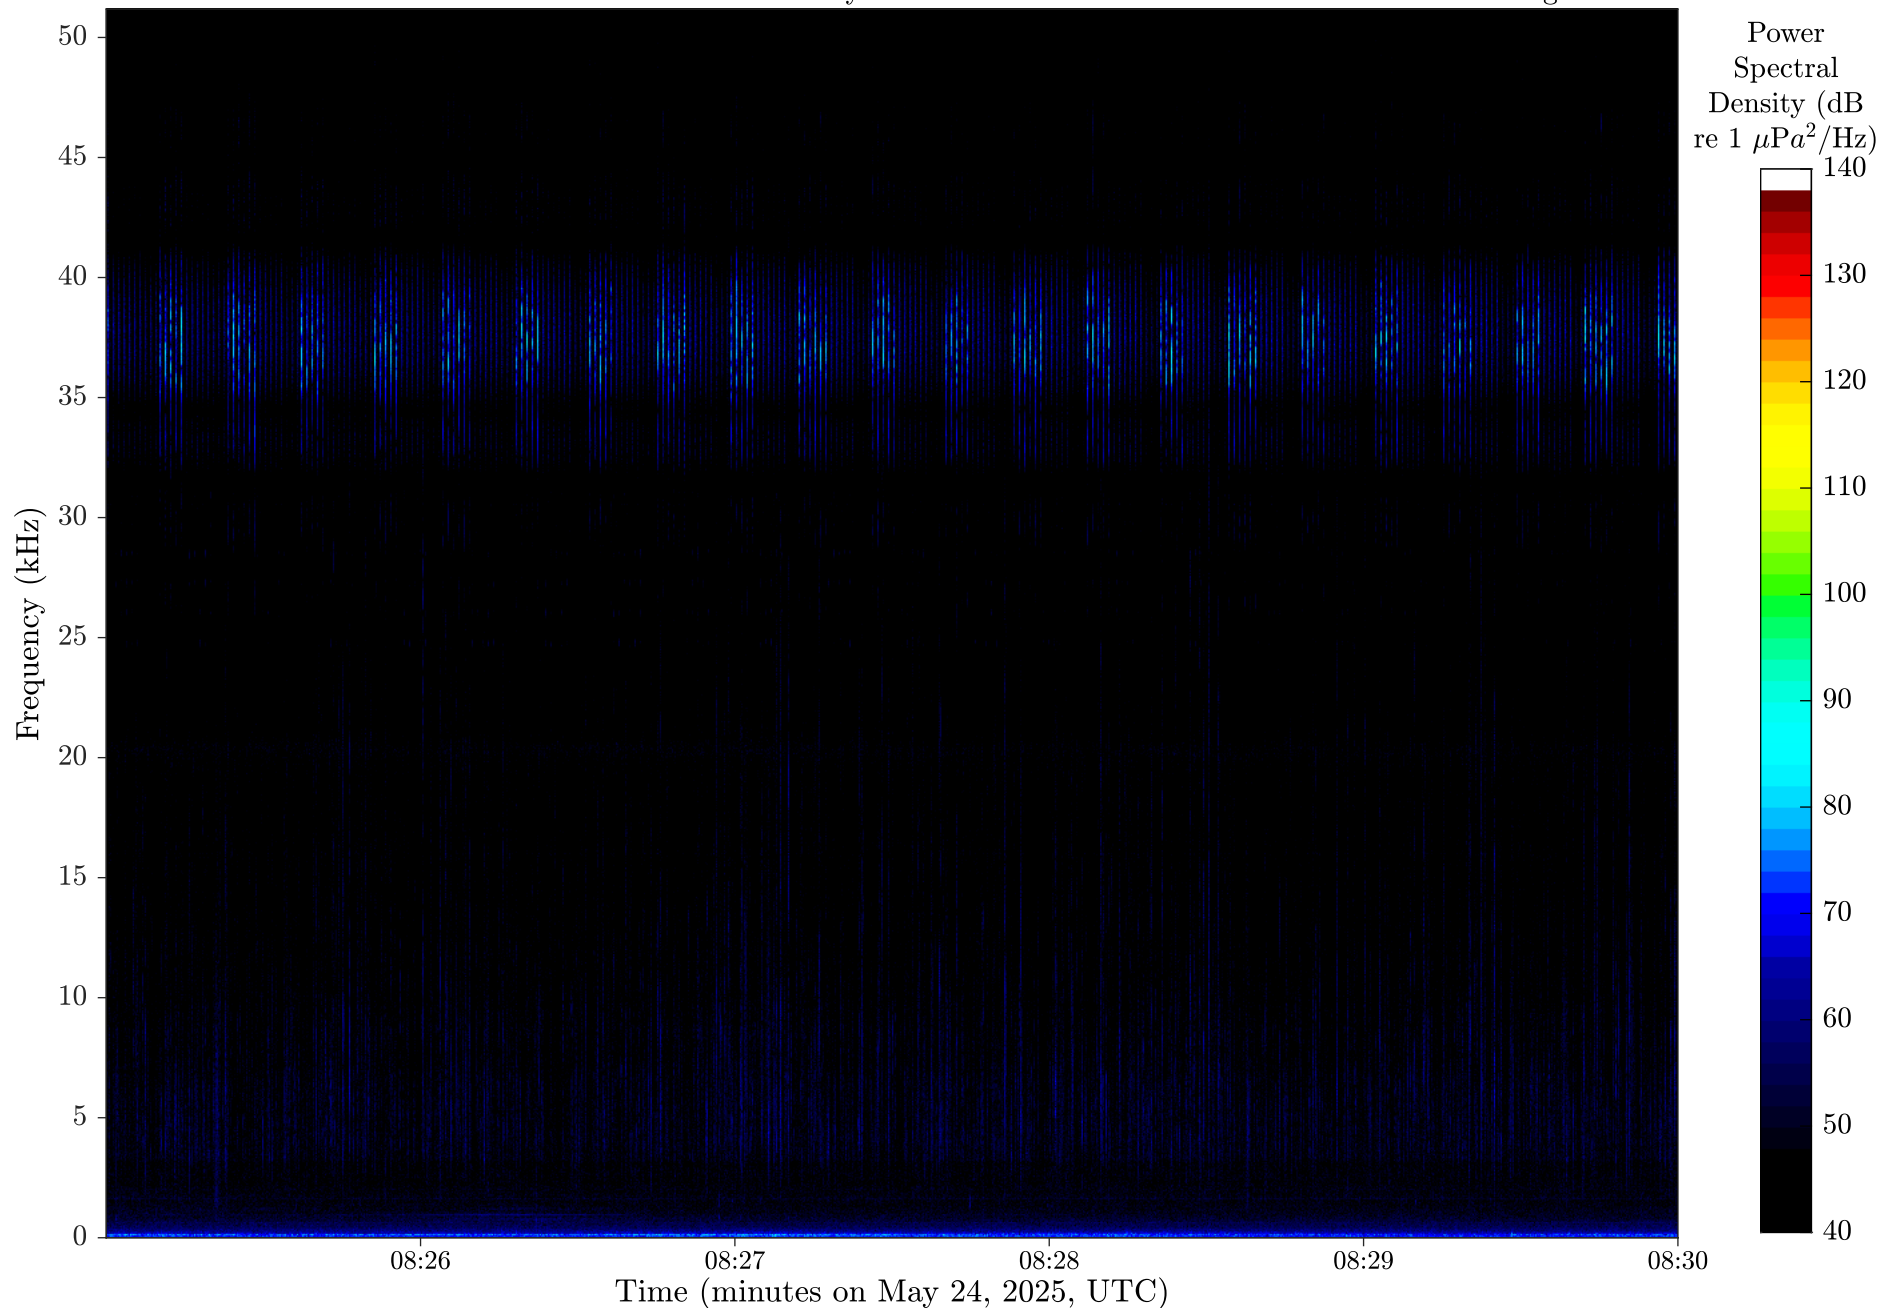

Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:29:04 UTC

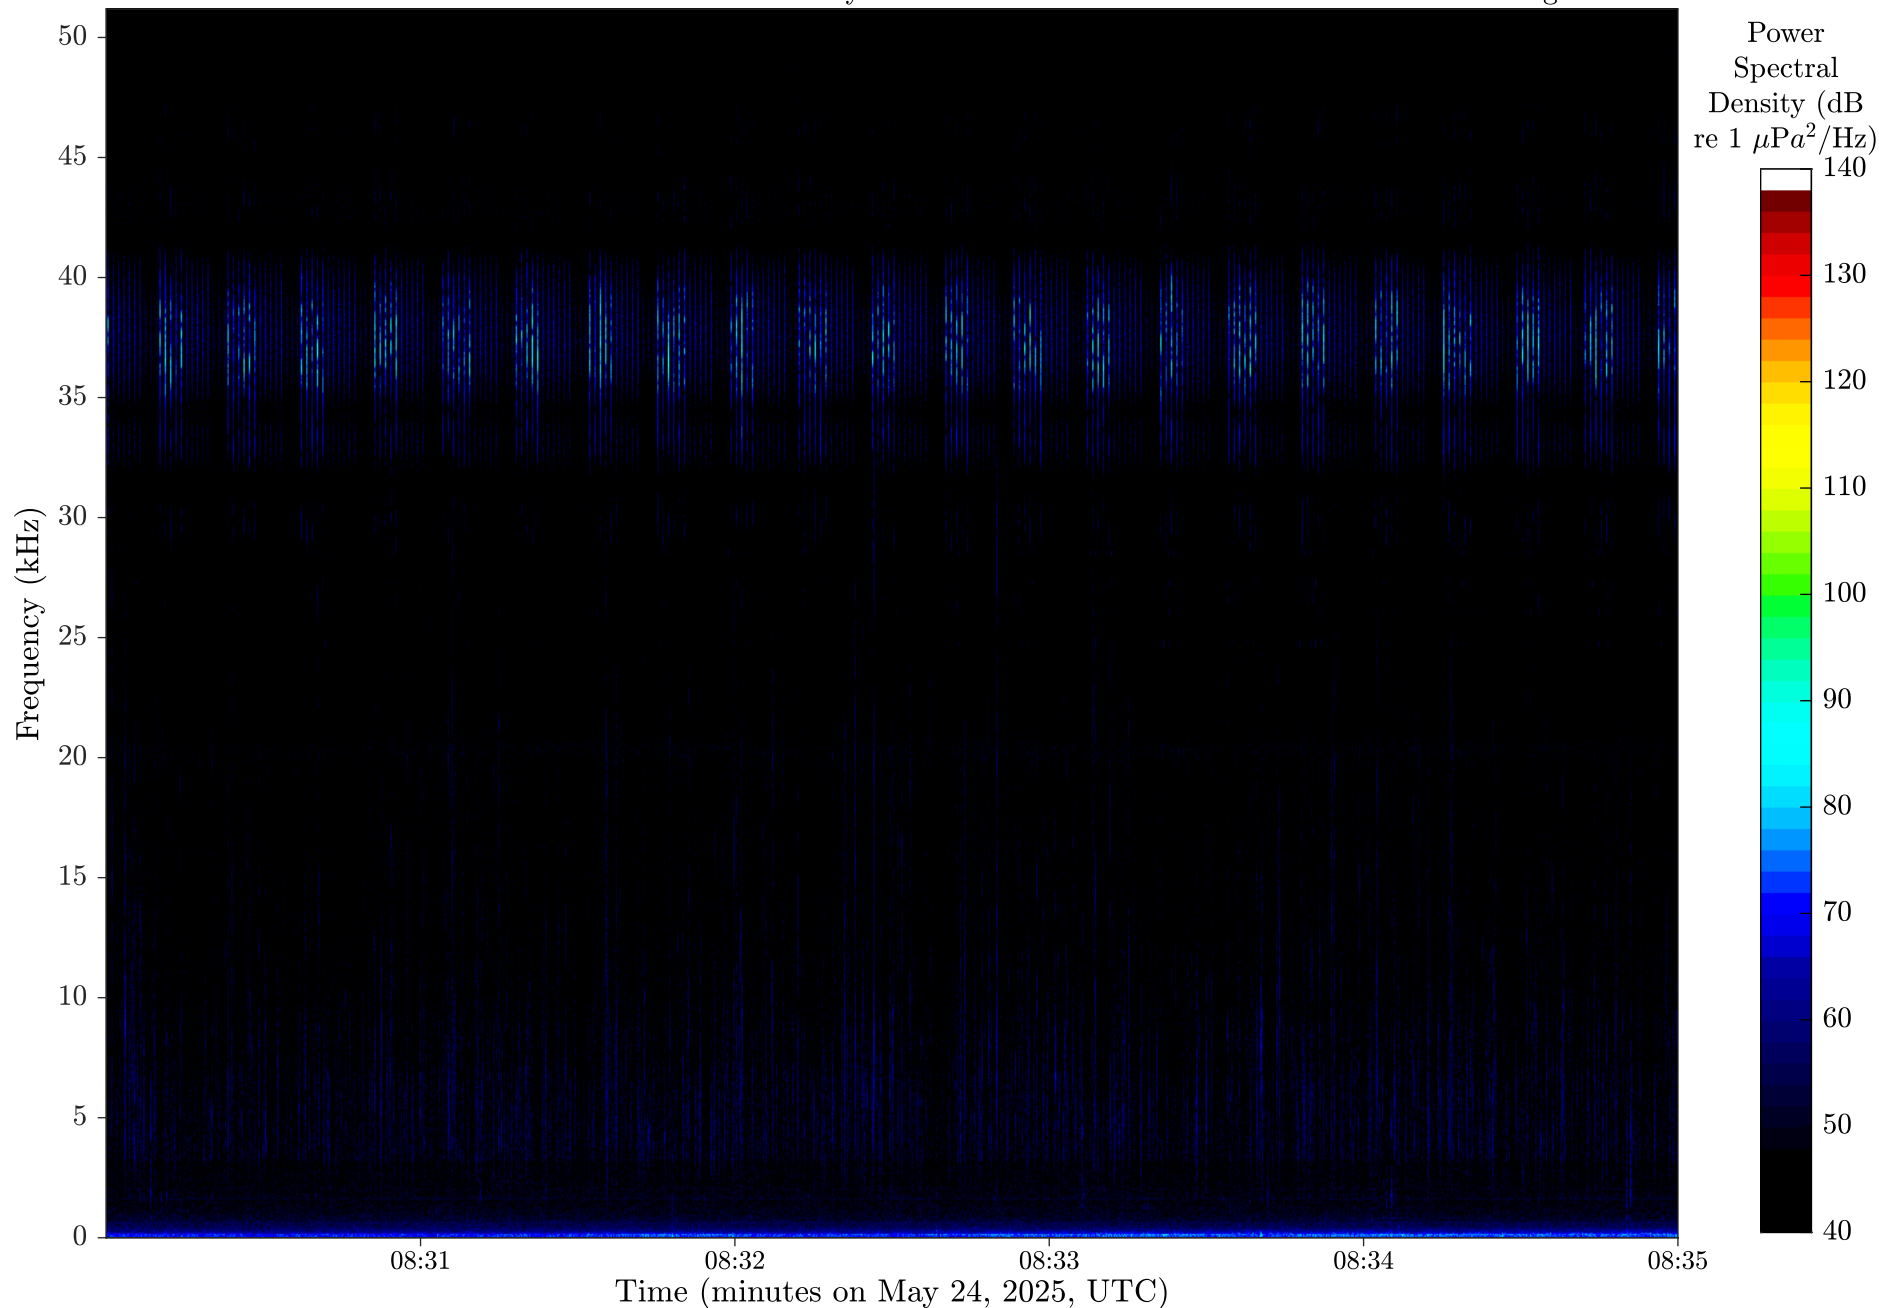


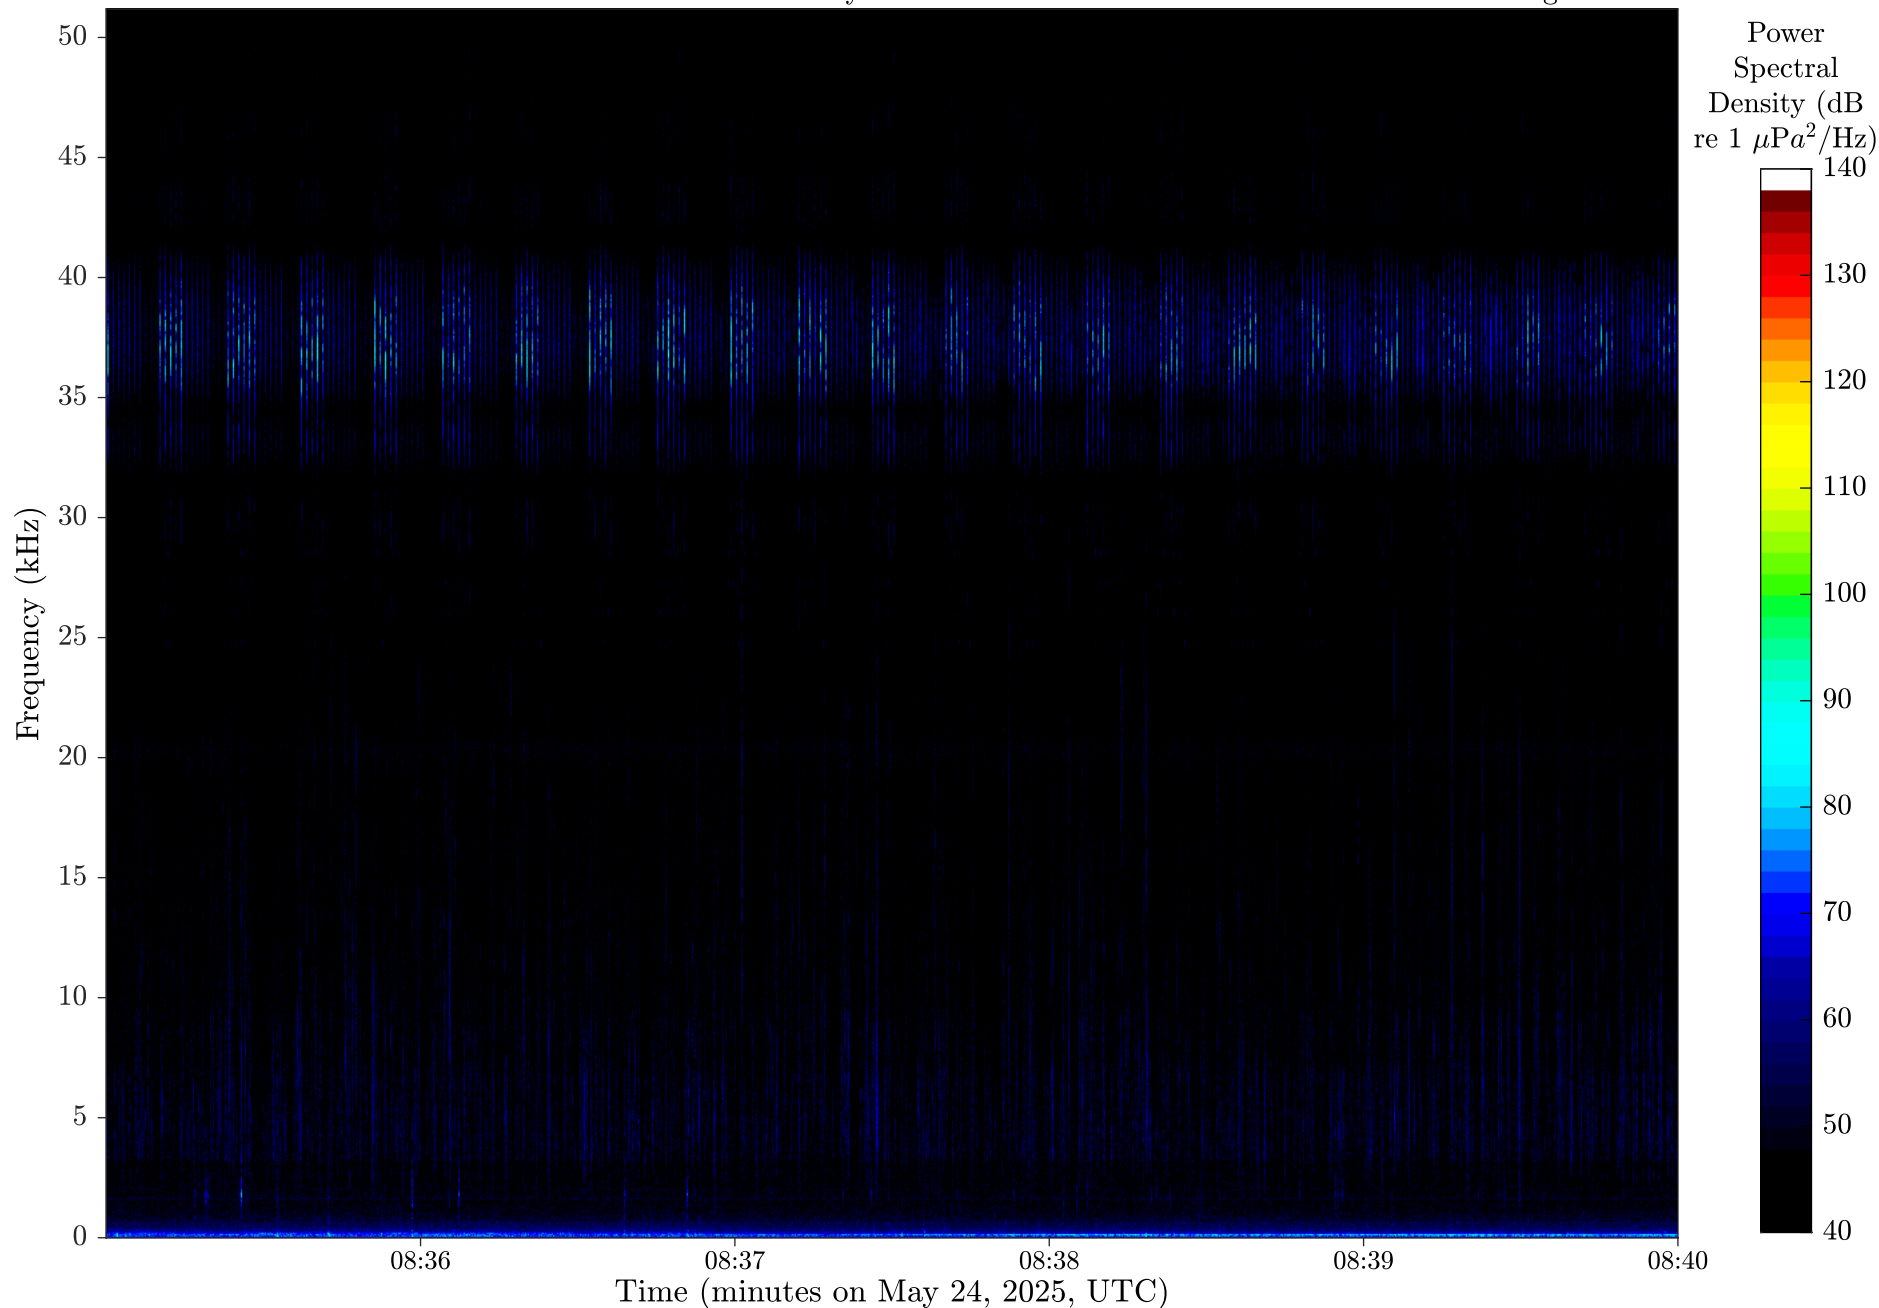

Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:29:19 UTC

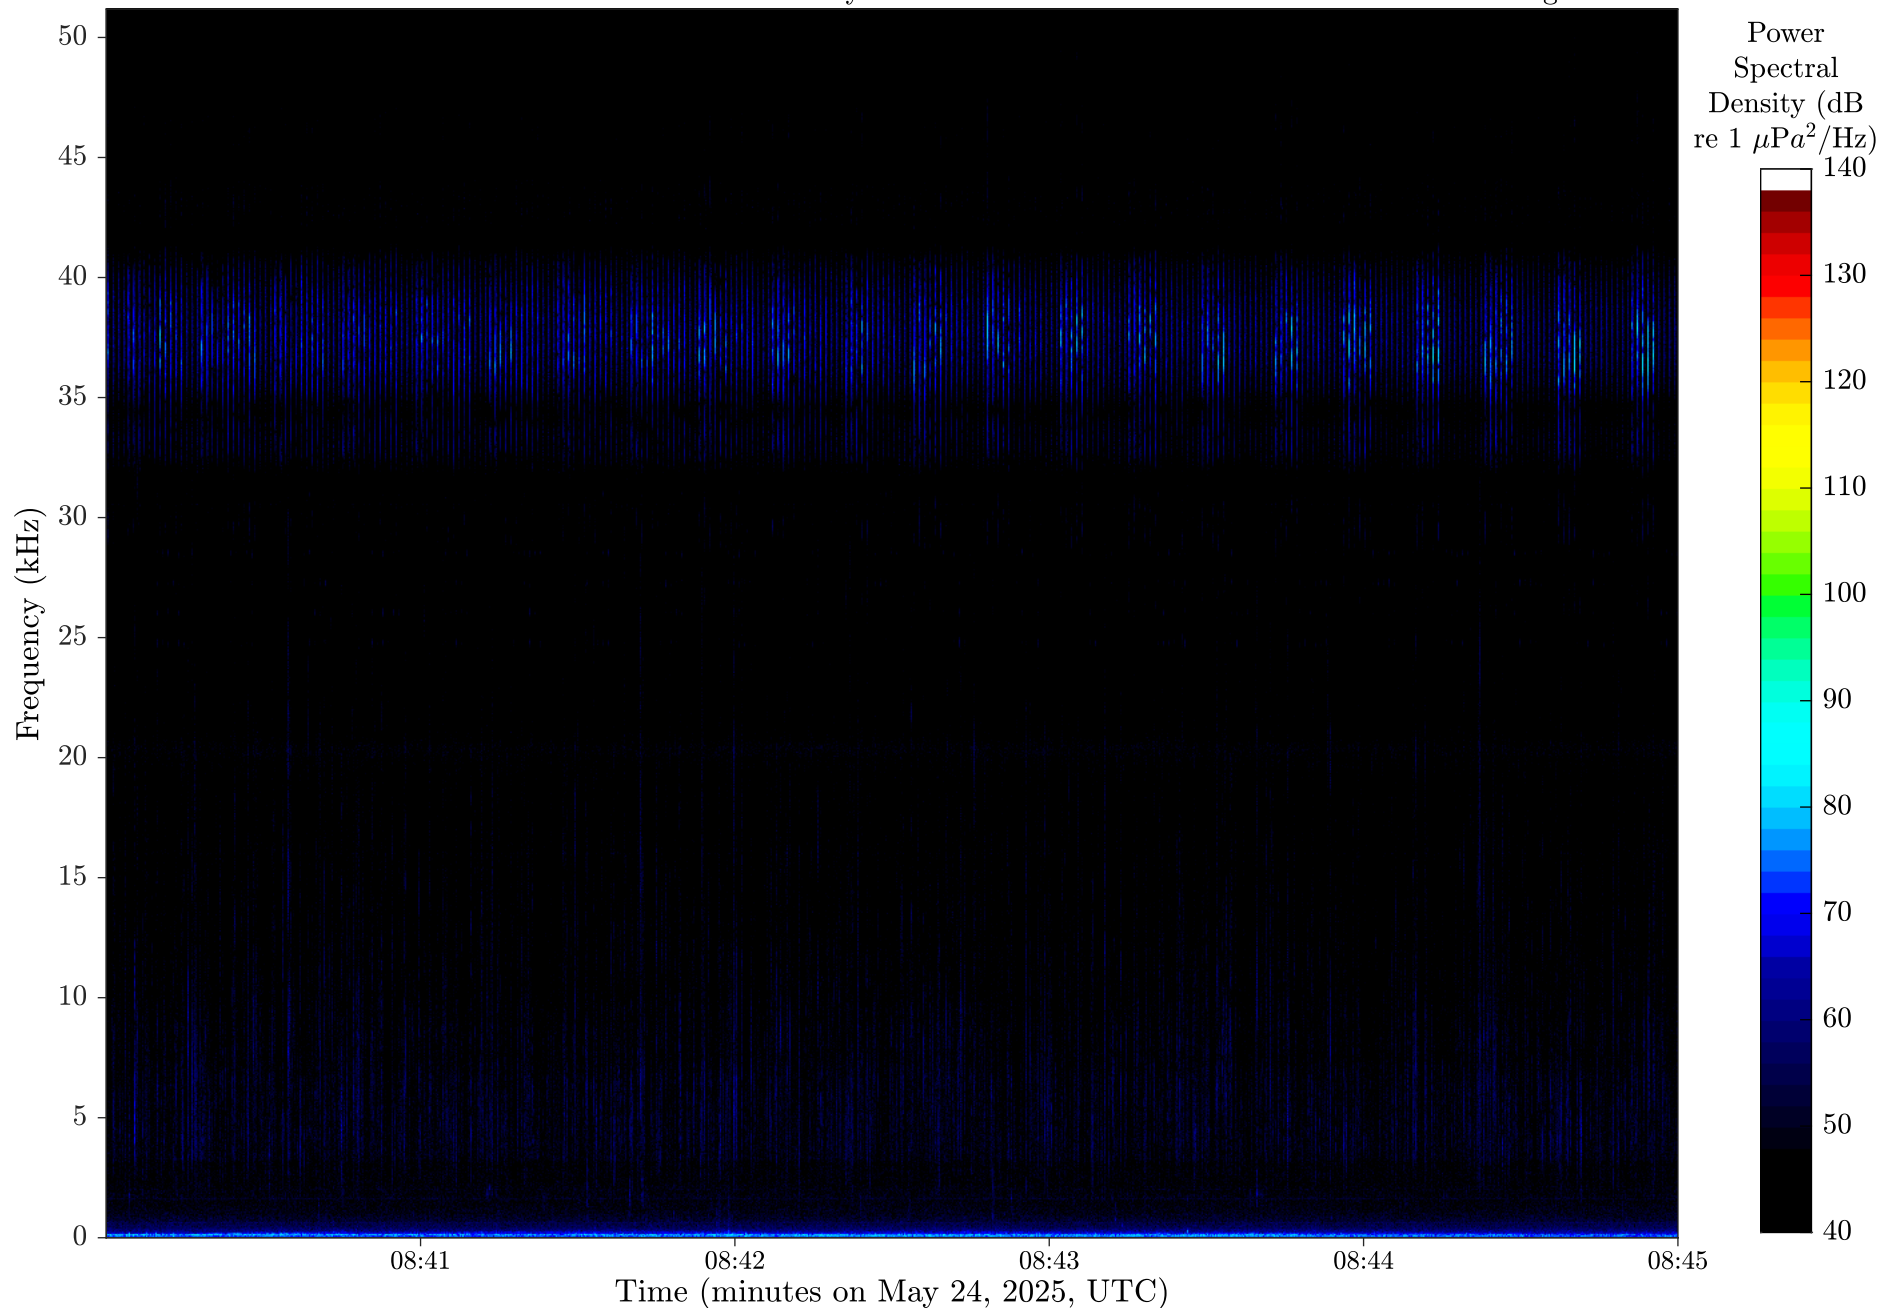

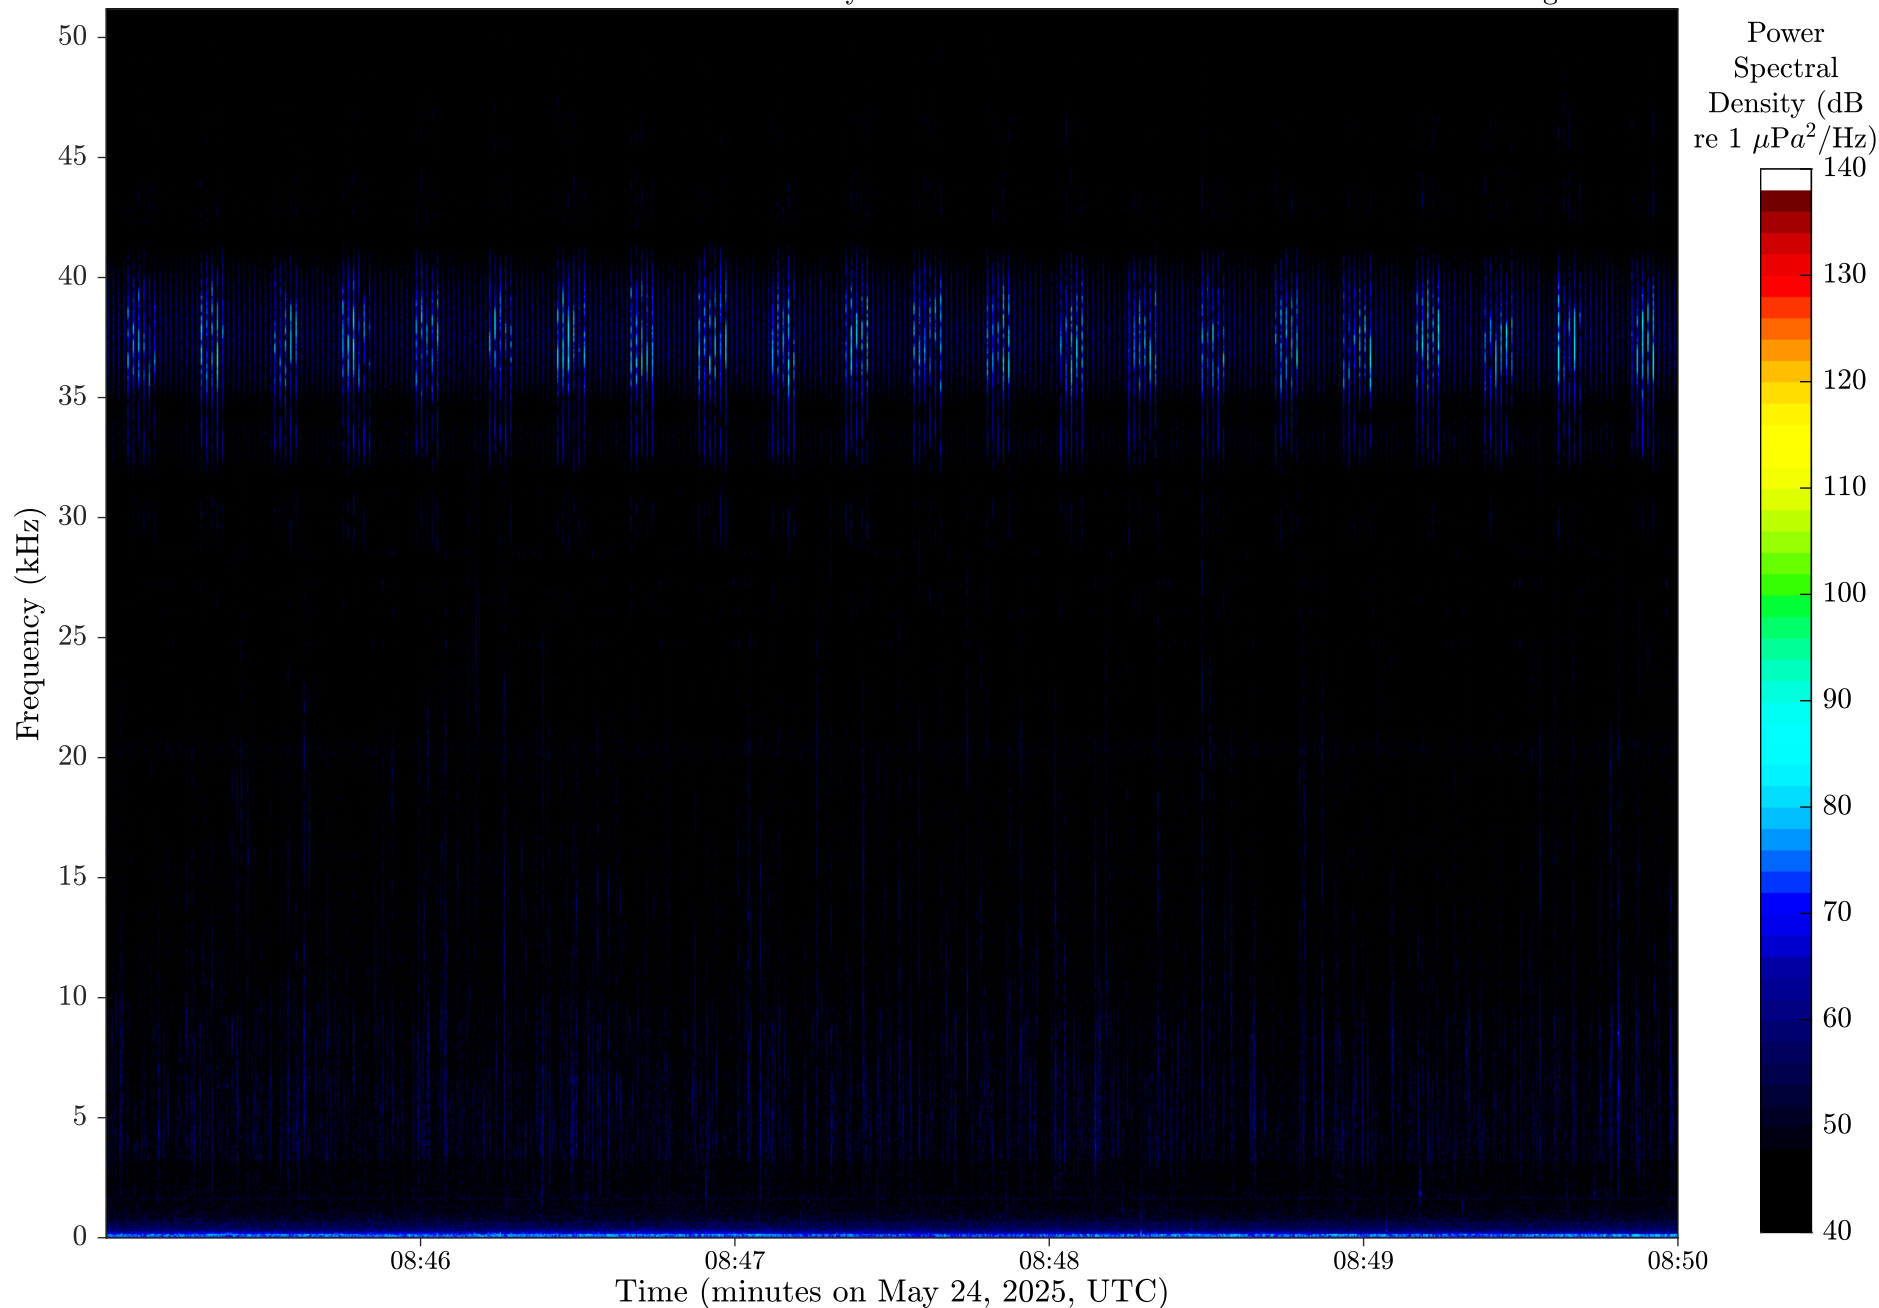


Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:35 UTC

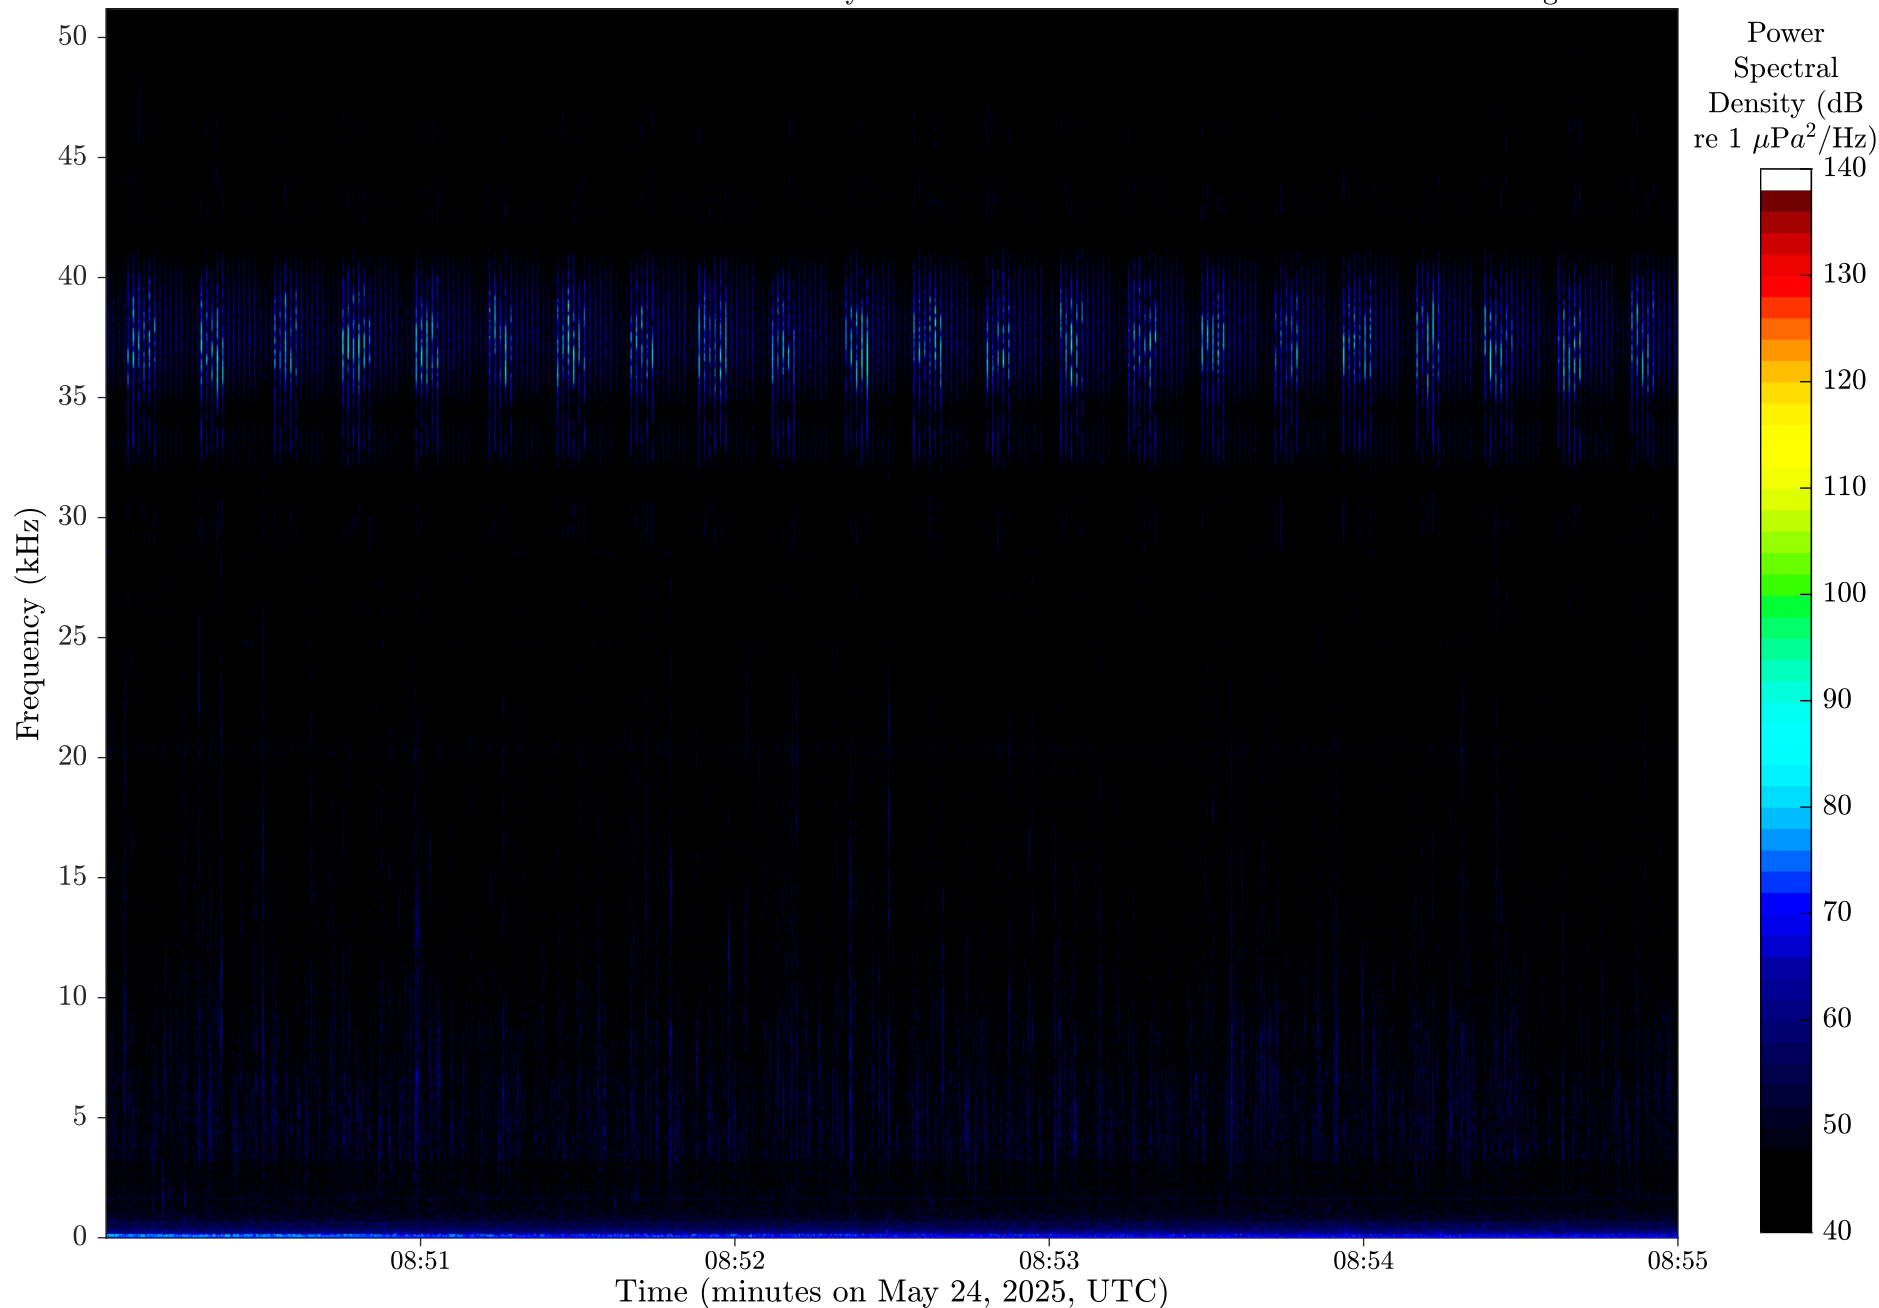


Comments: 36.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:43 UTC

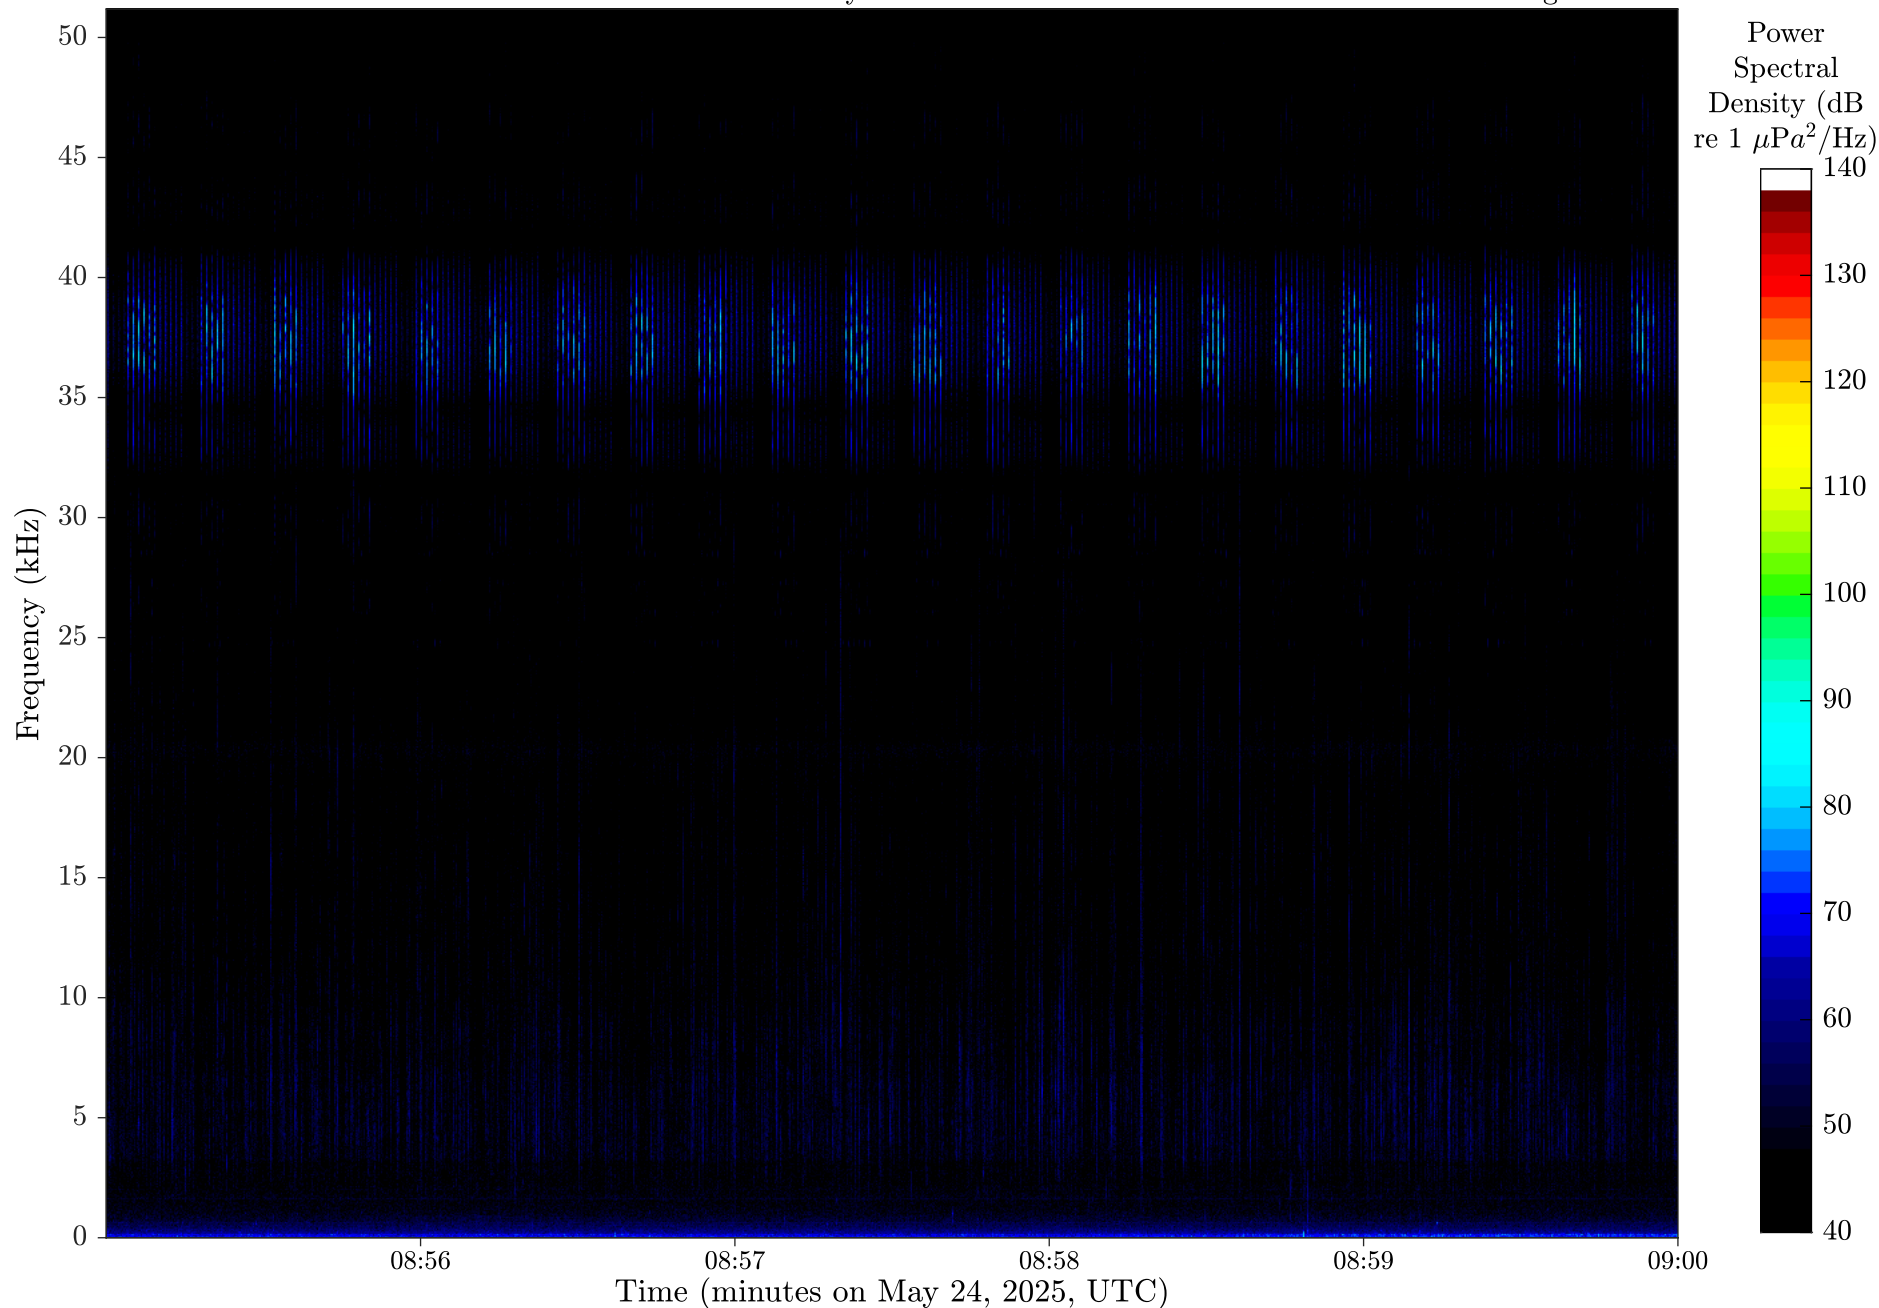


Comments: 36.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:51 UTC

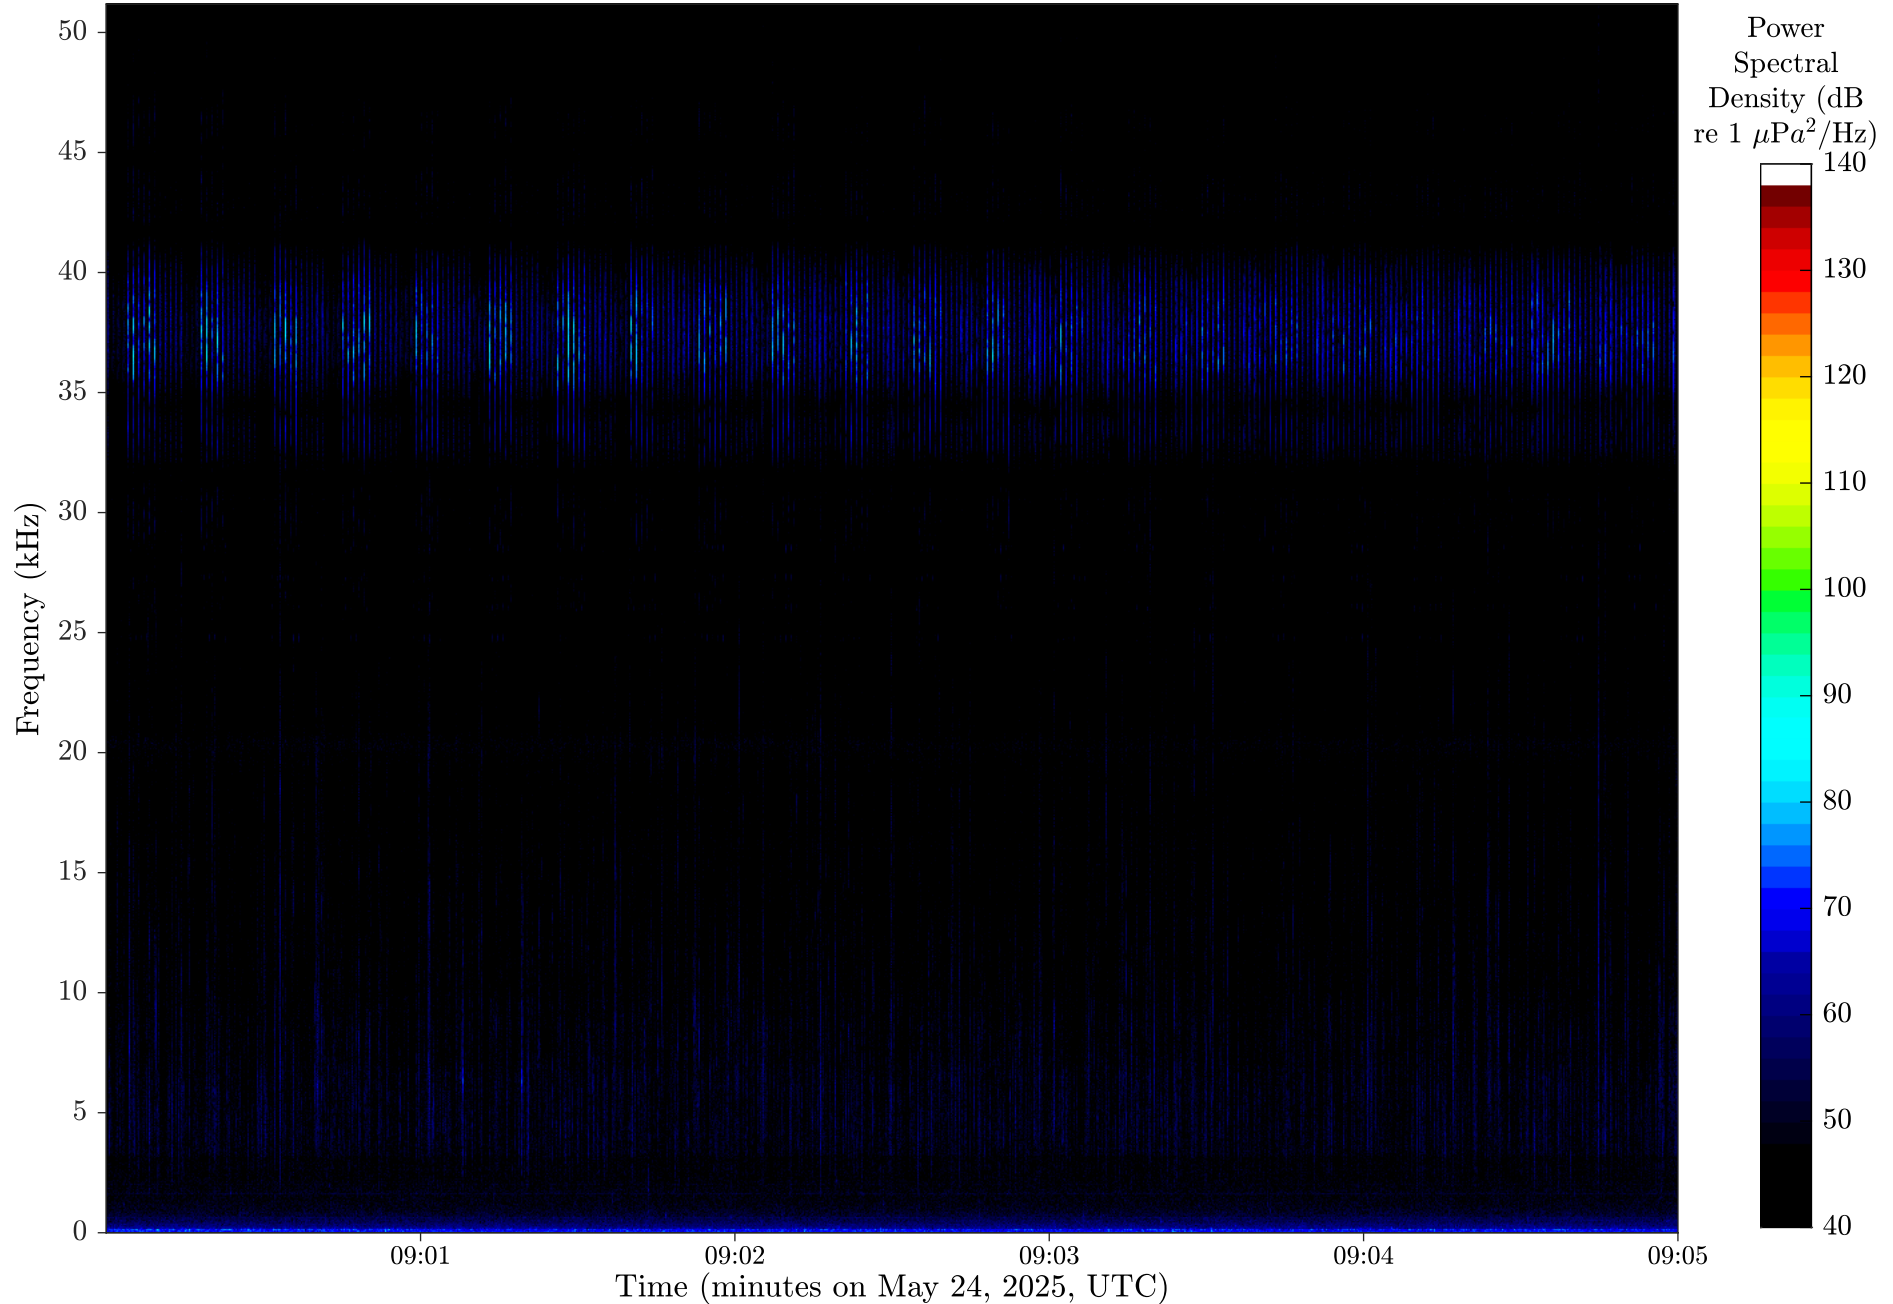


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:59 UTC

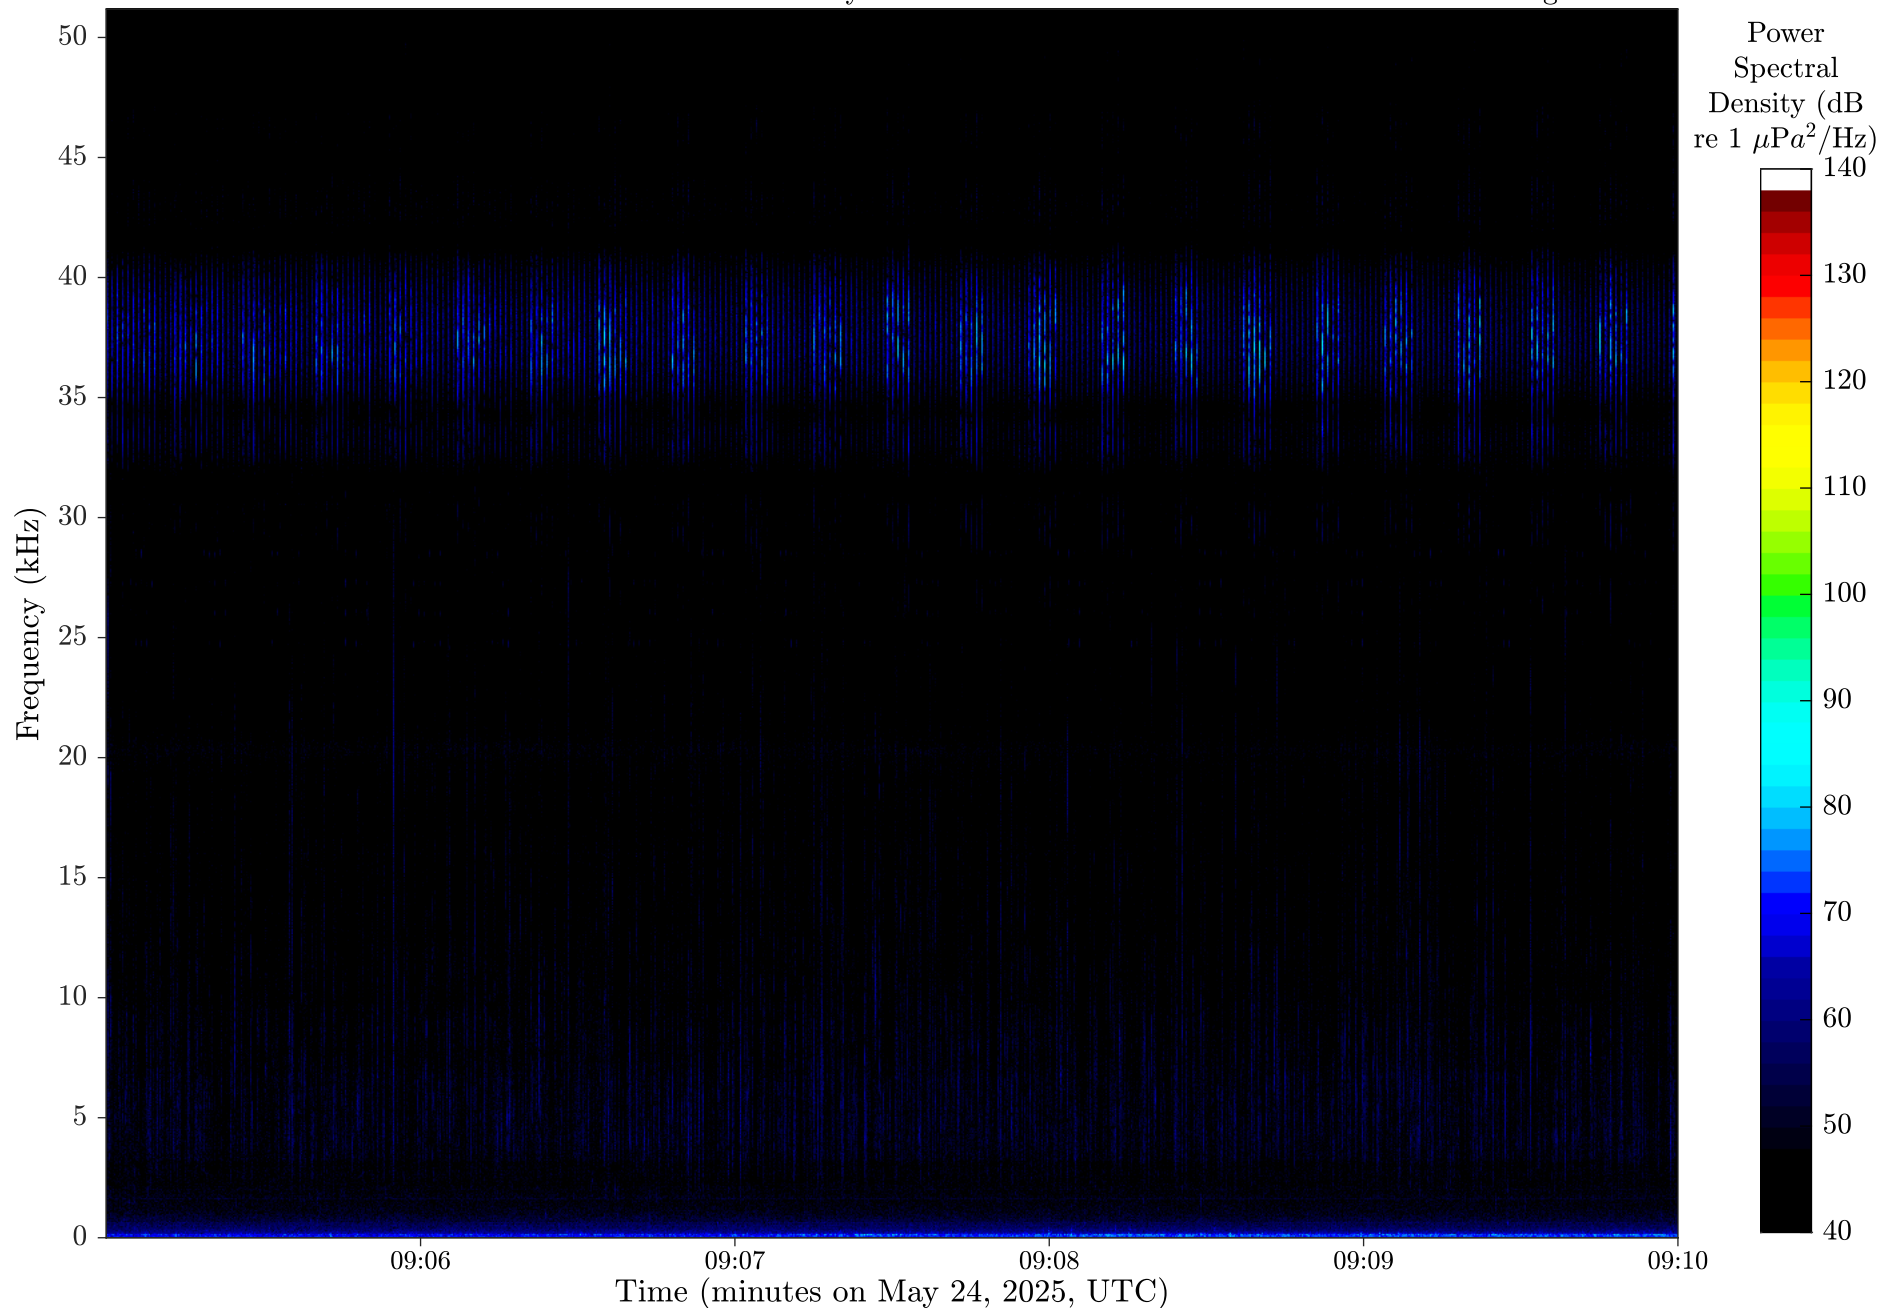


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:30:07 UTC

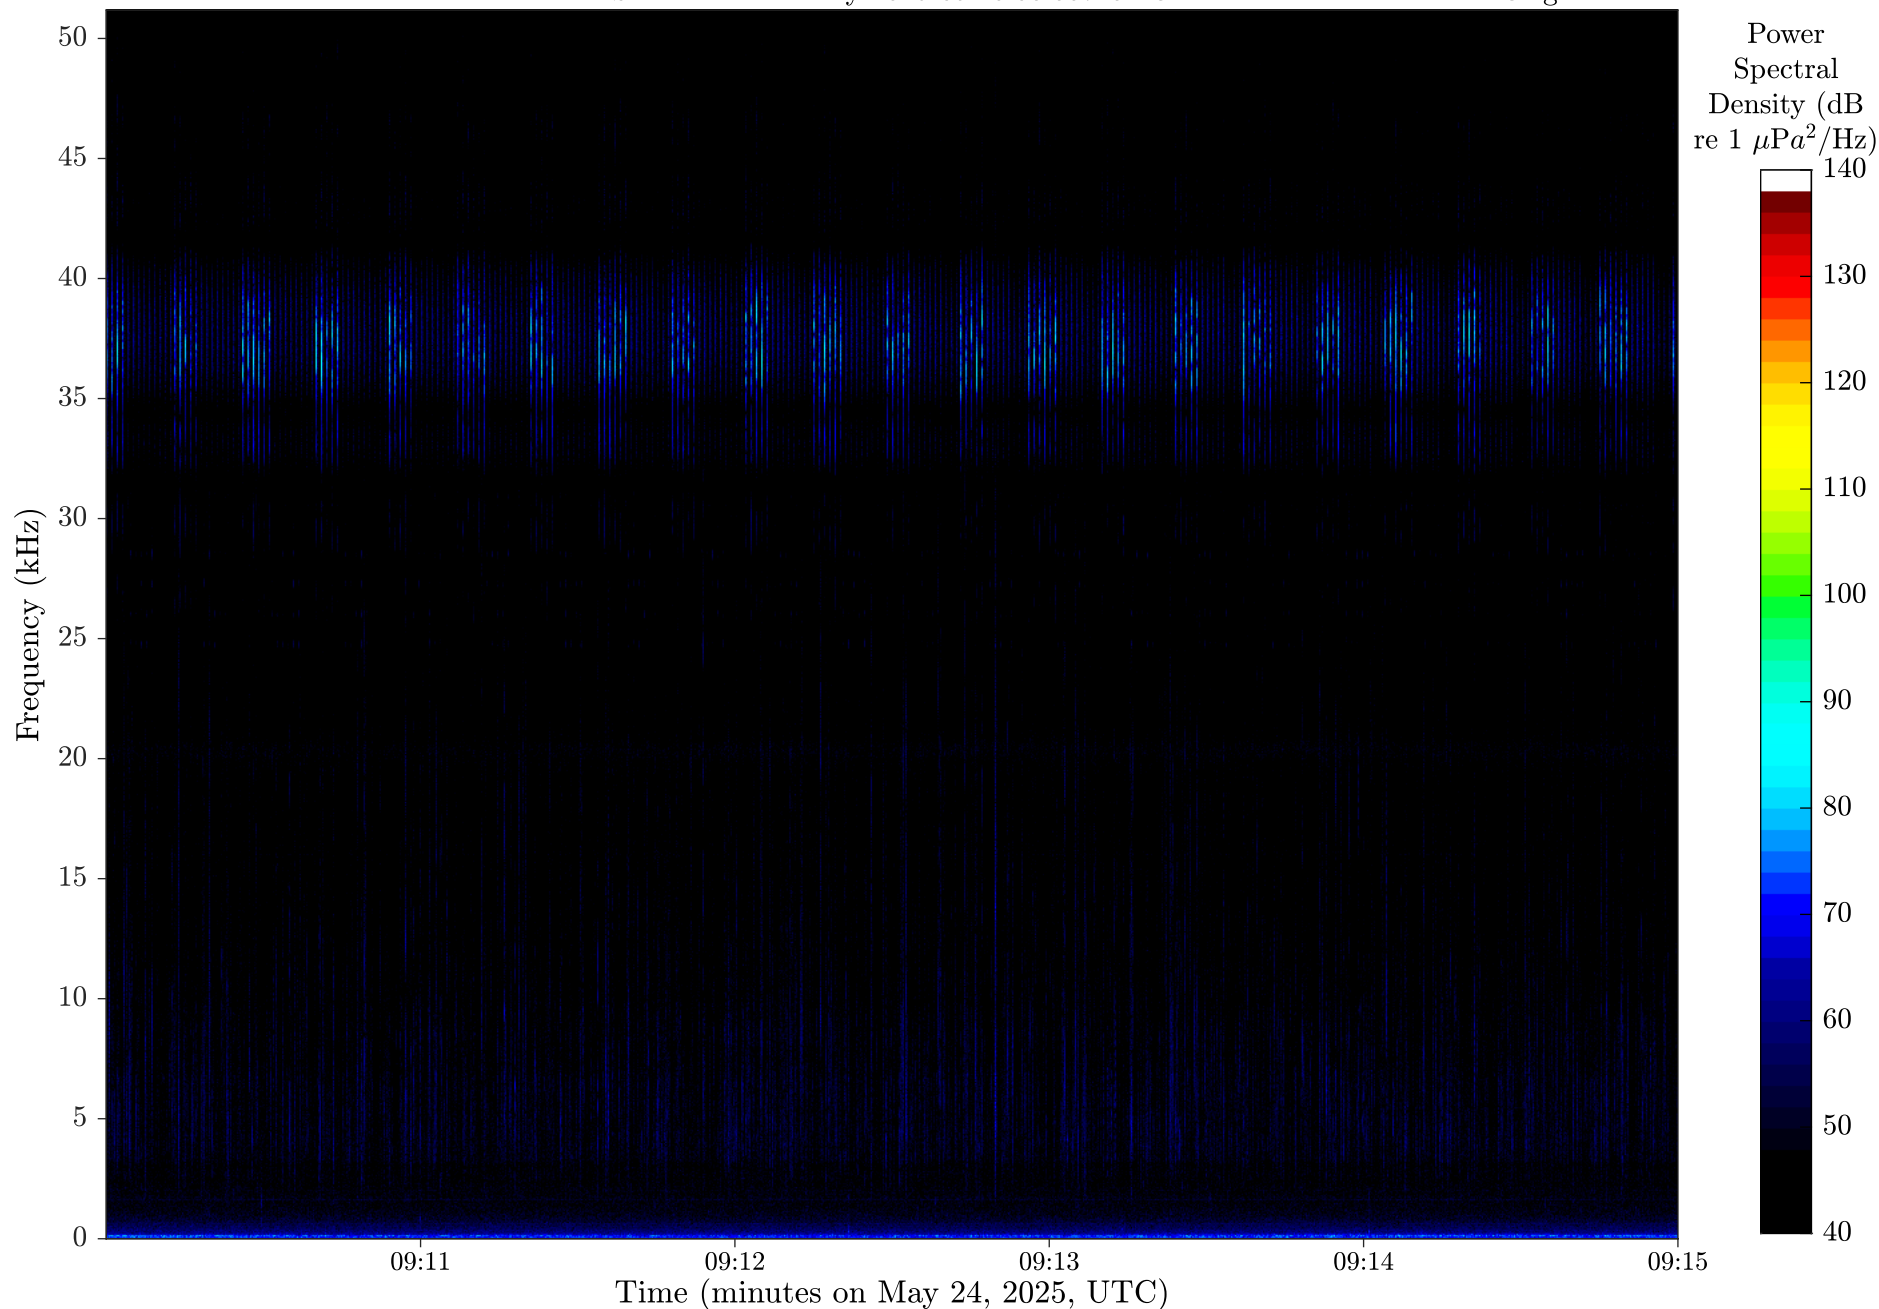


Comments: 35.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:30:16 UTC

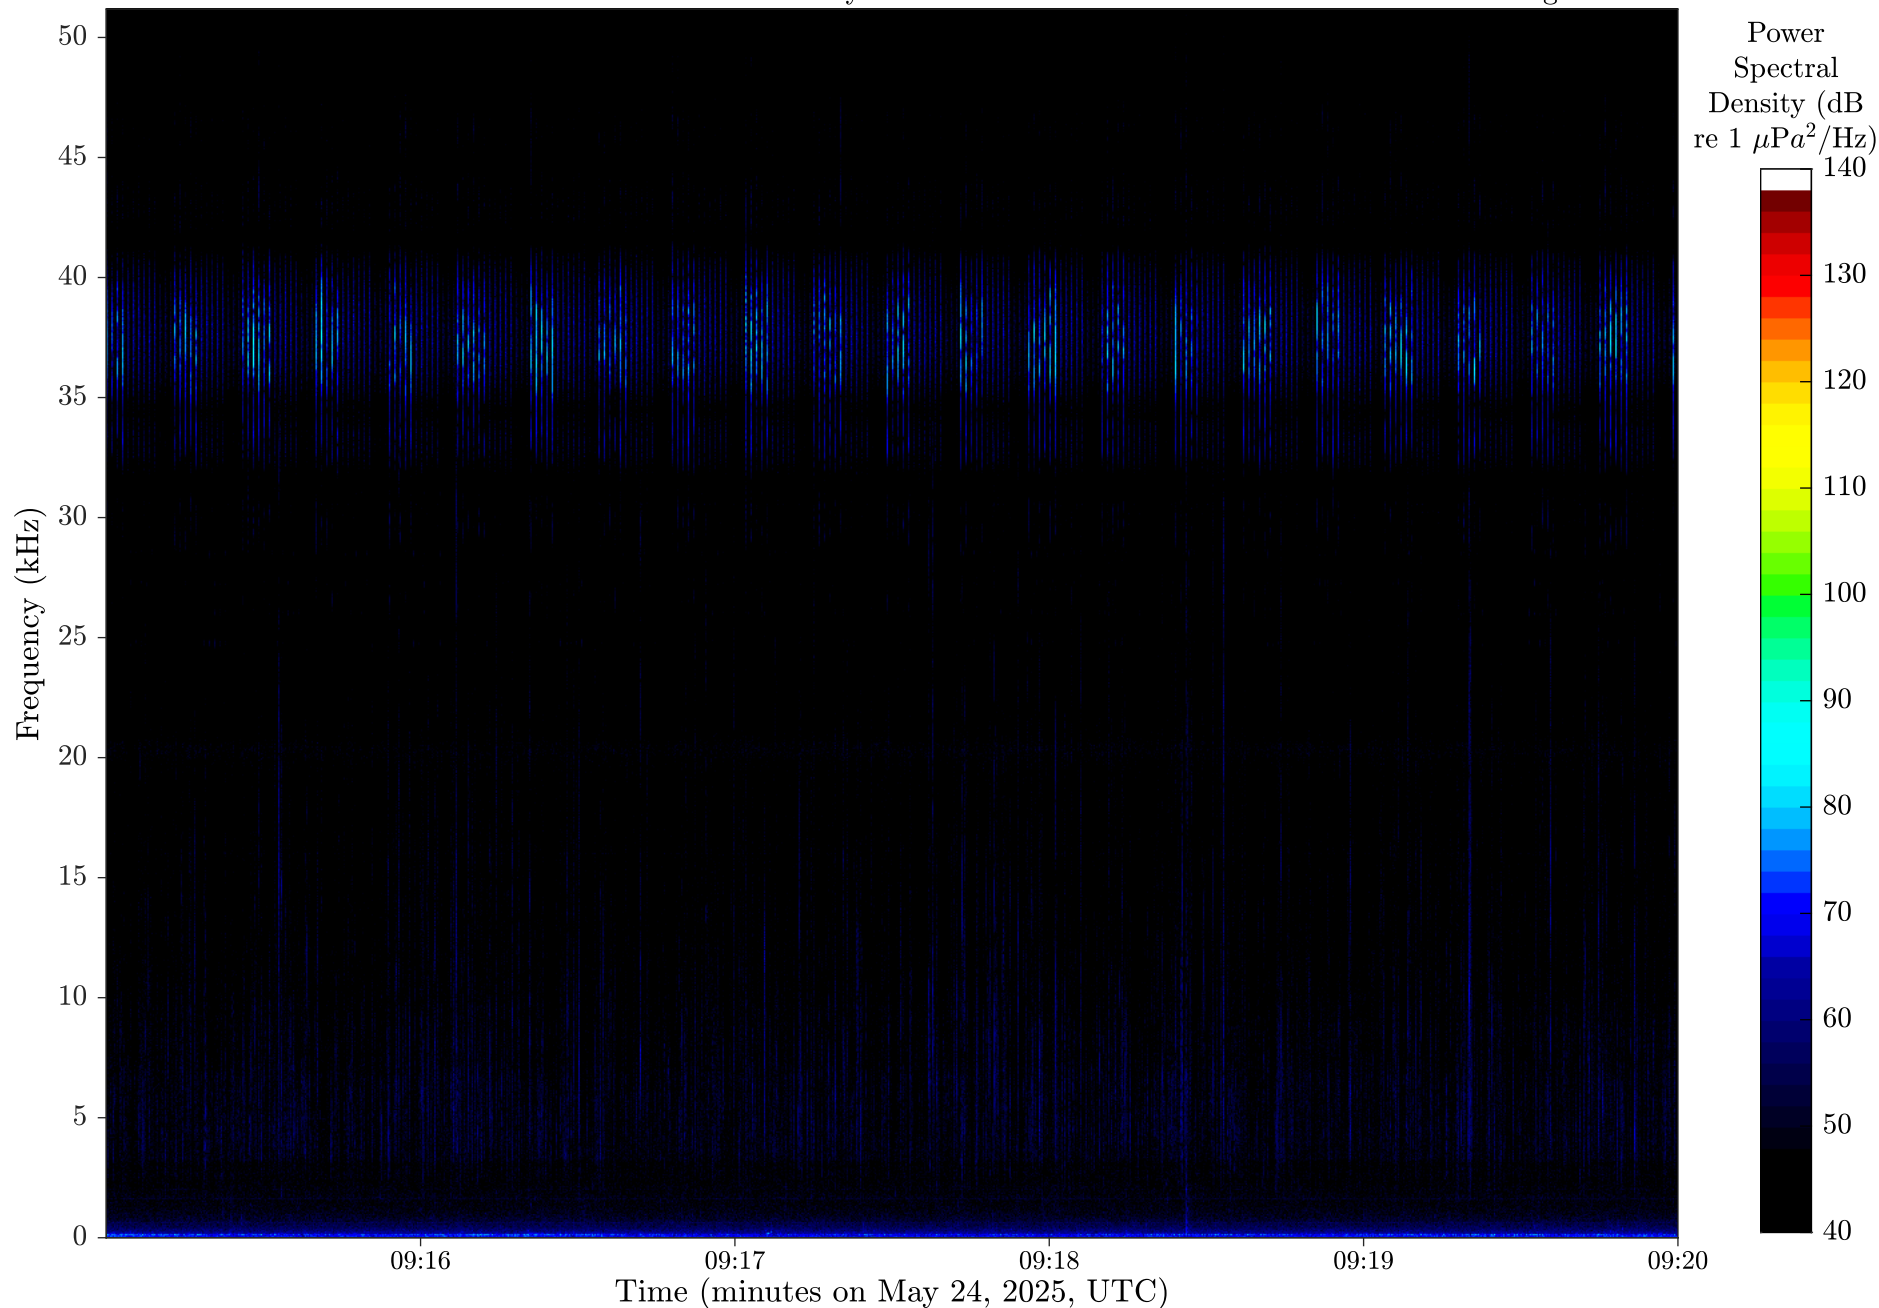


Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:30:24 UTC

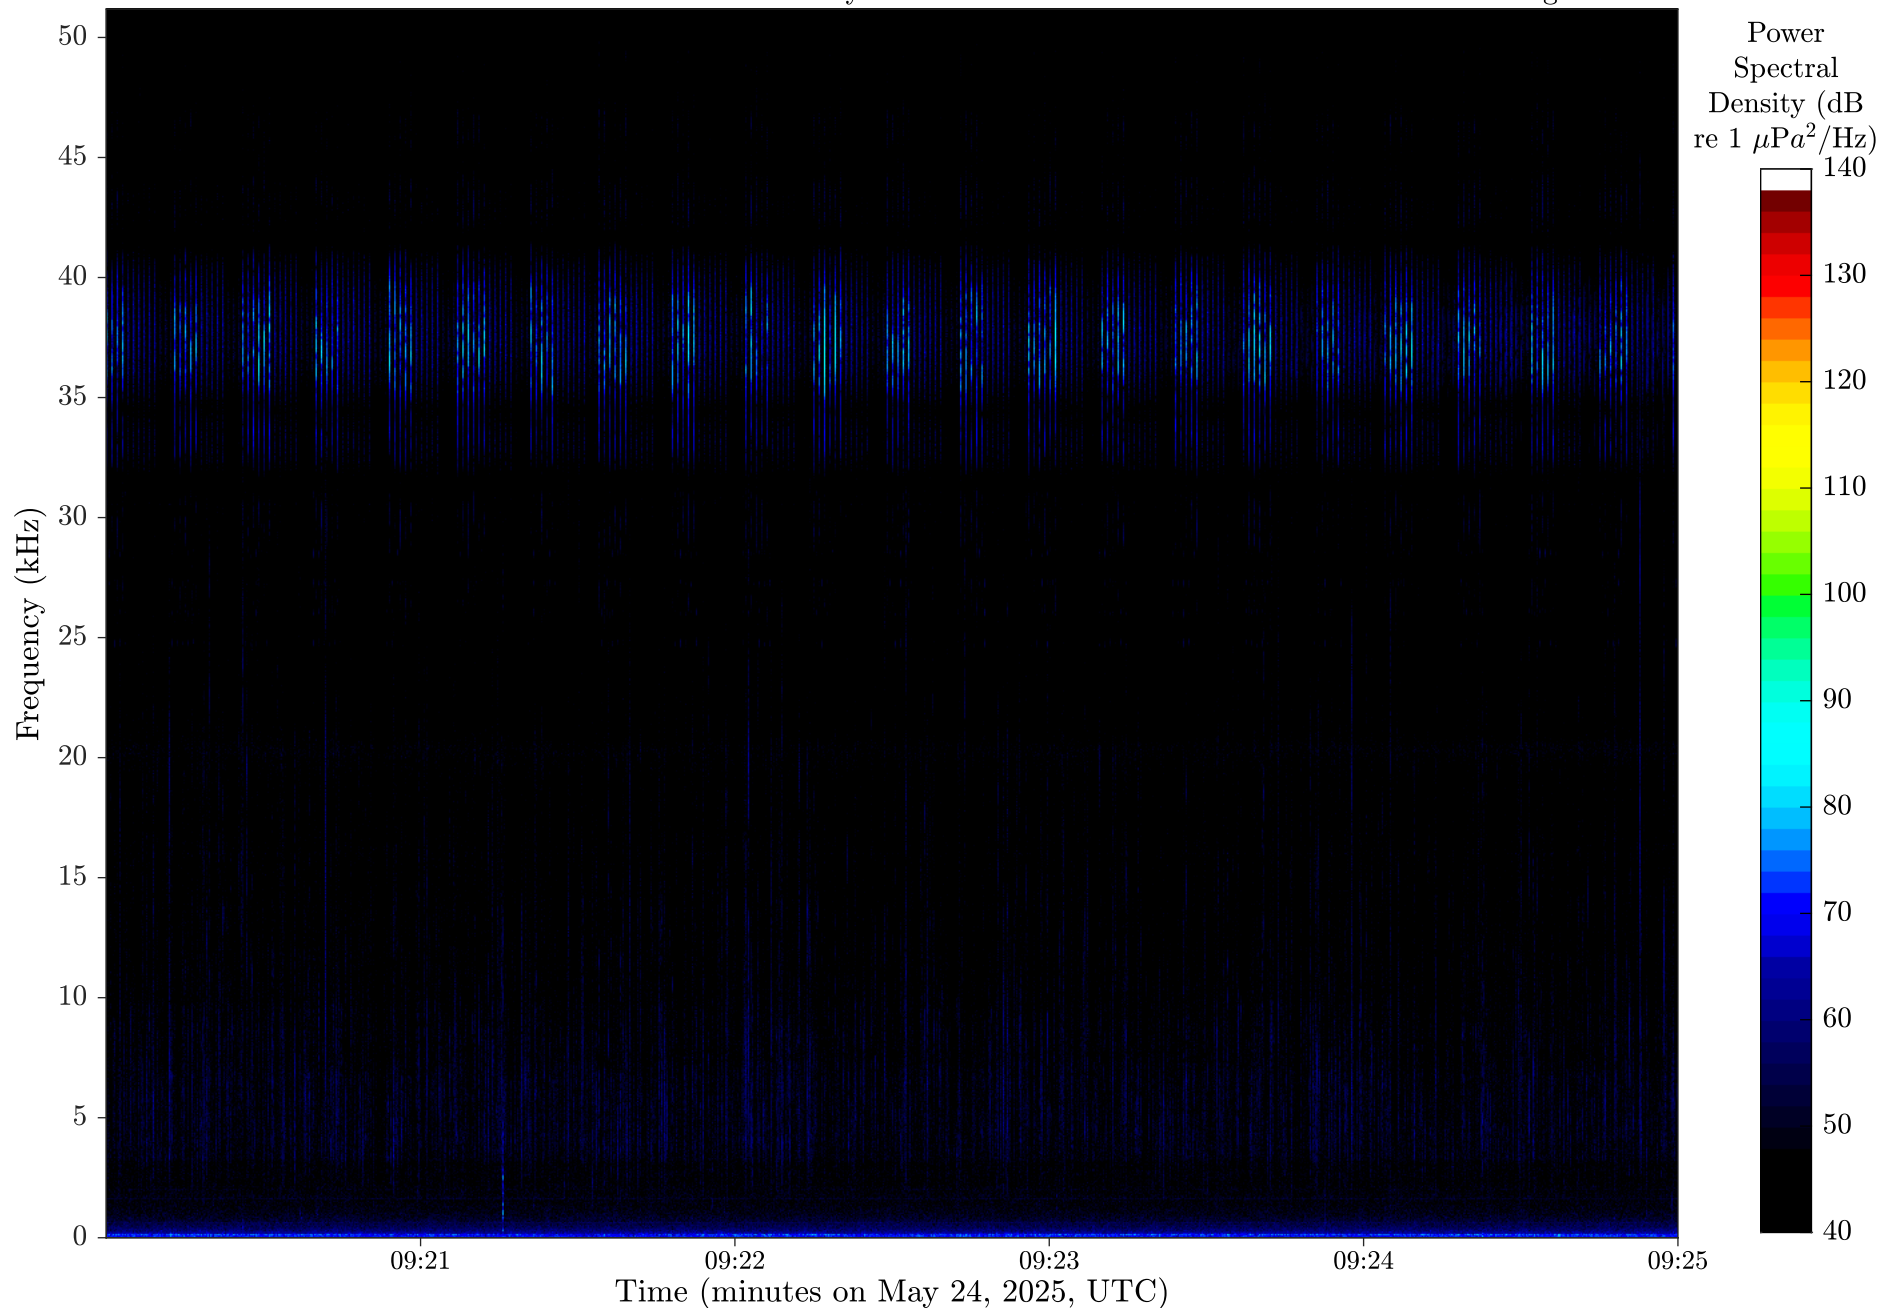


Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:30:33 UTC

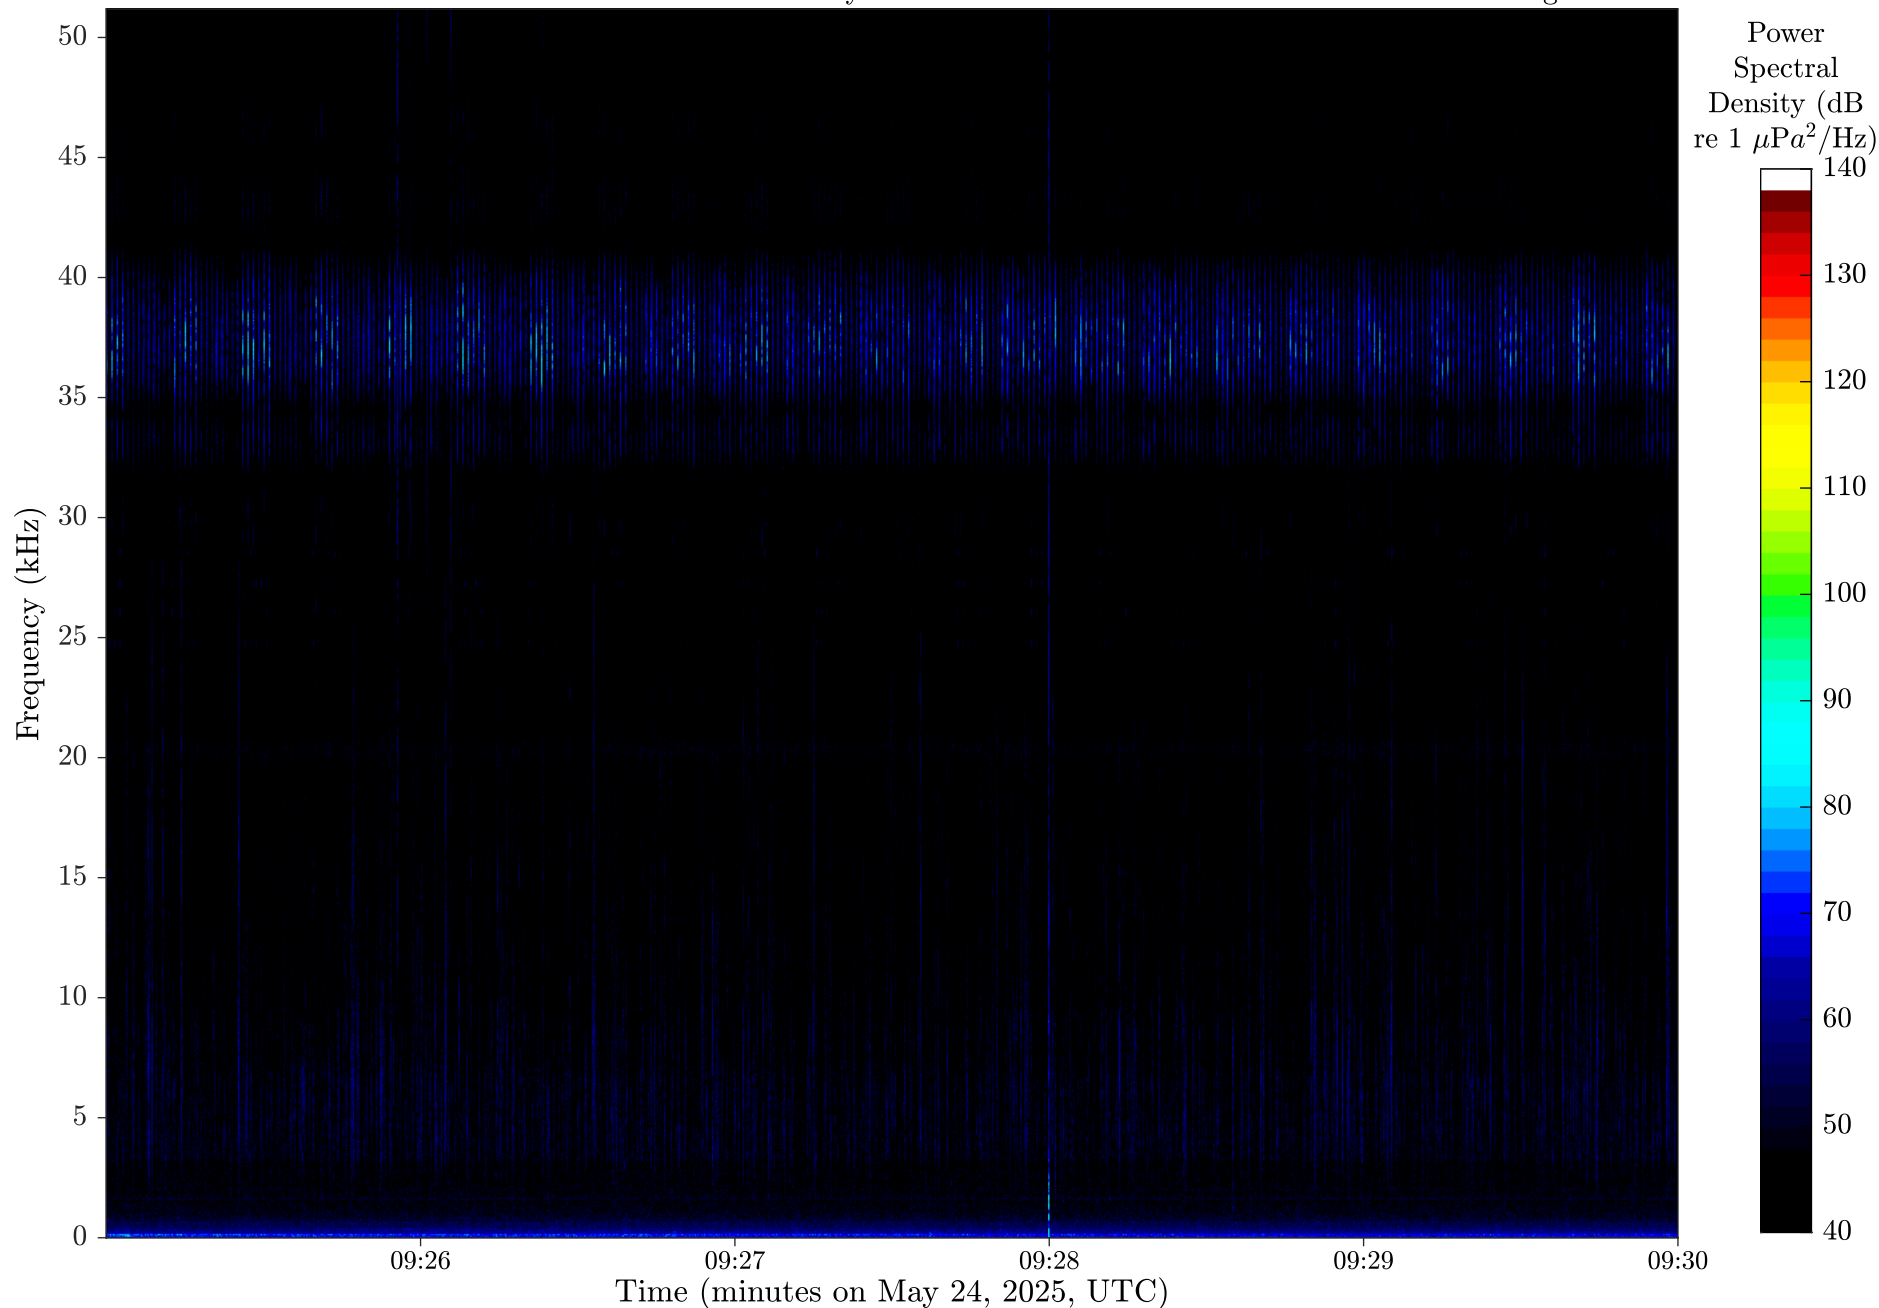


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:30:42 UTC

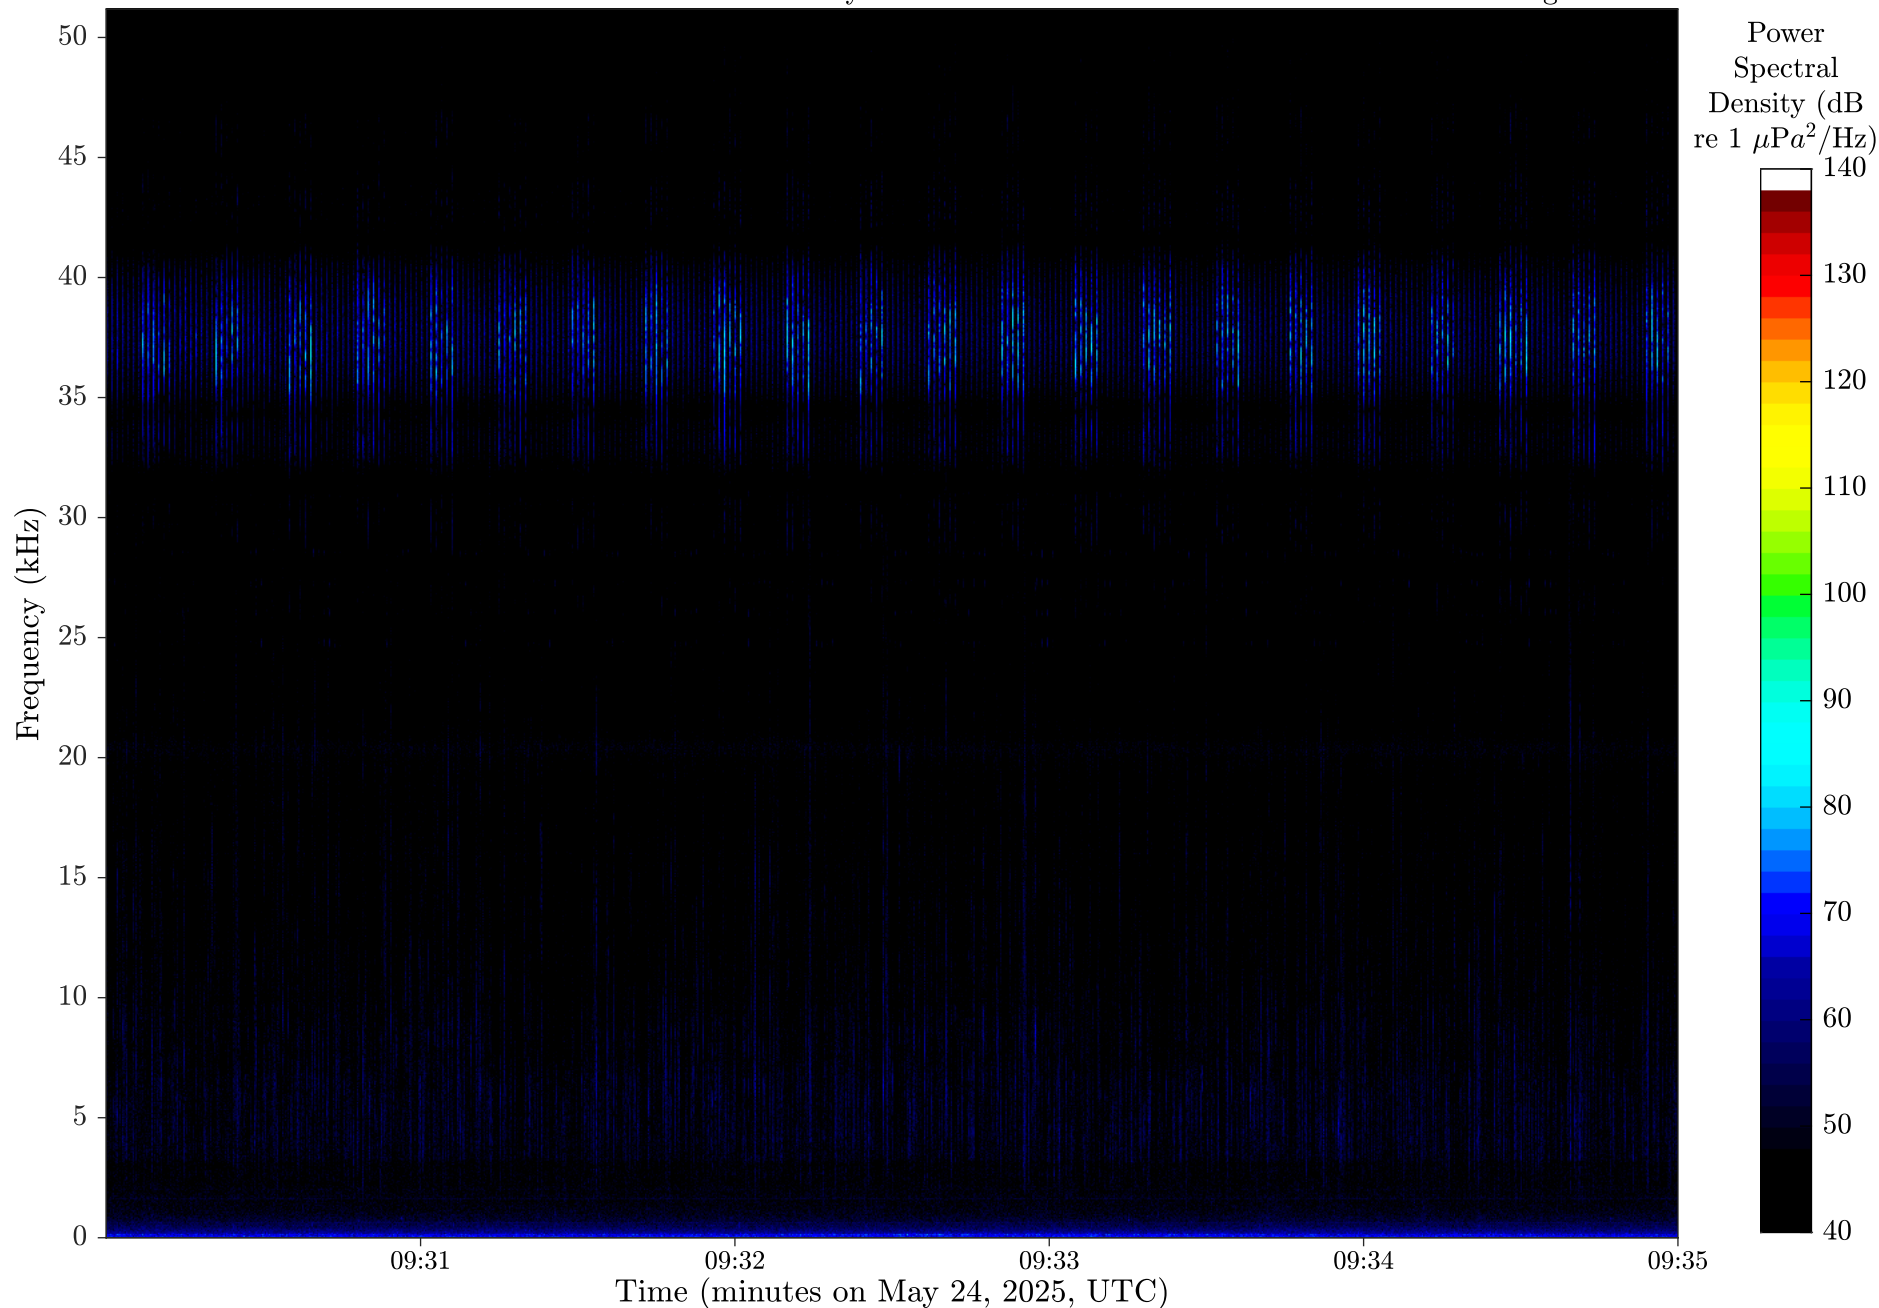

Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:30:51 UTC

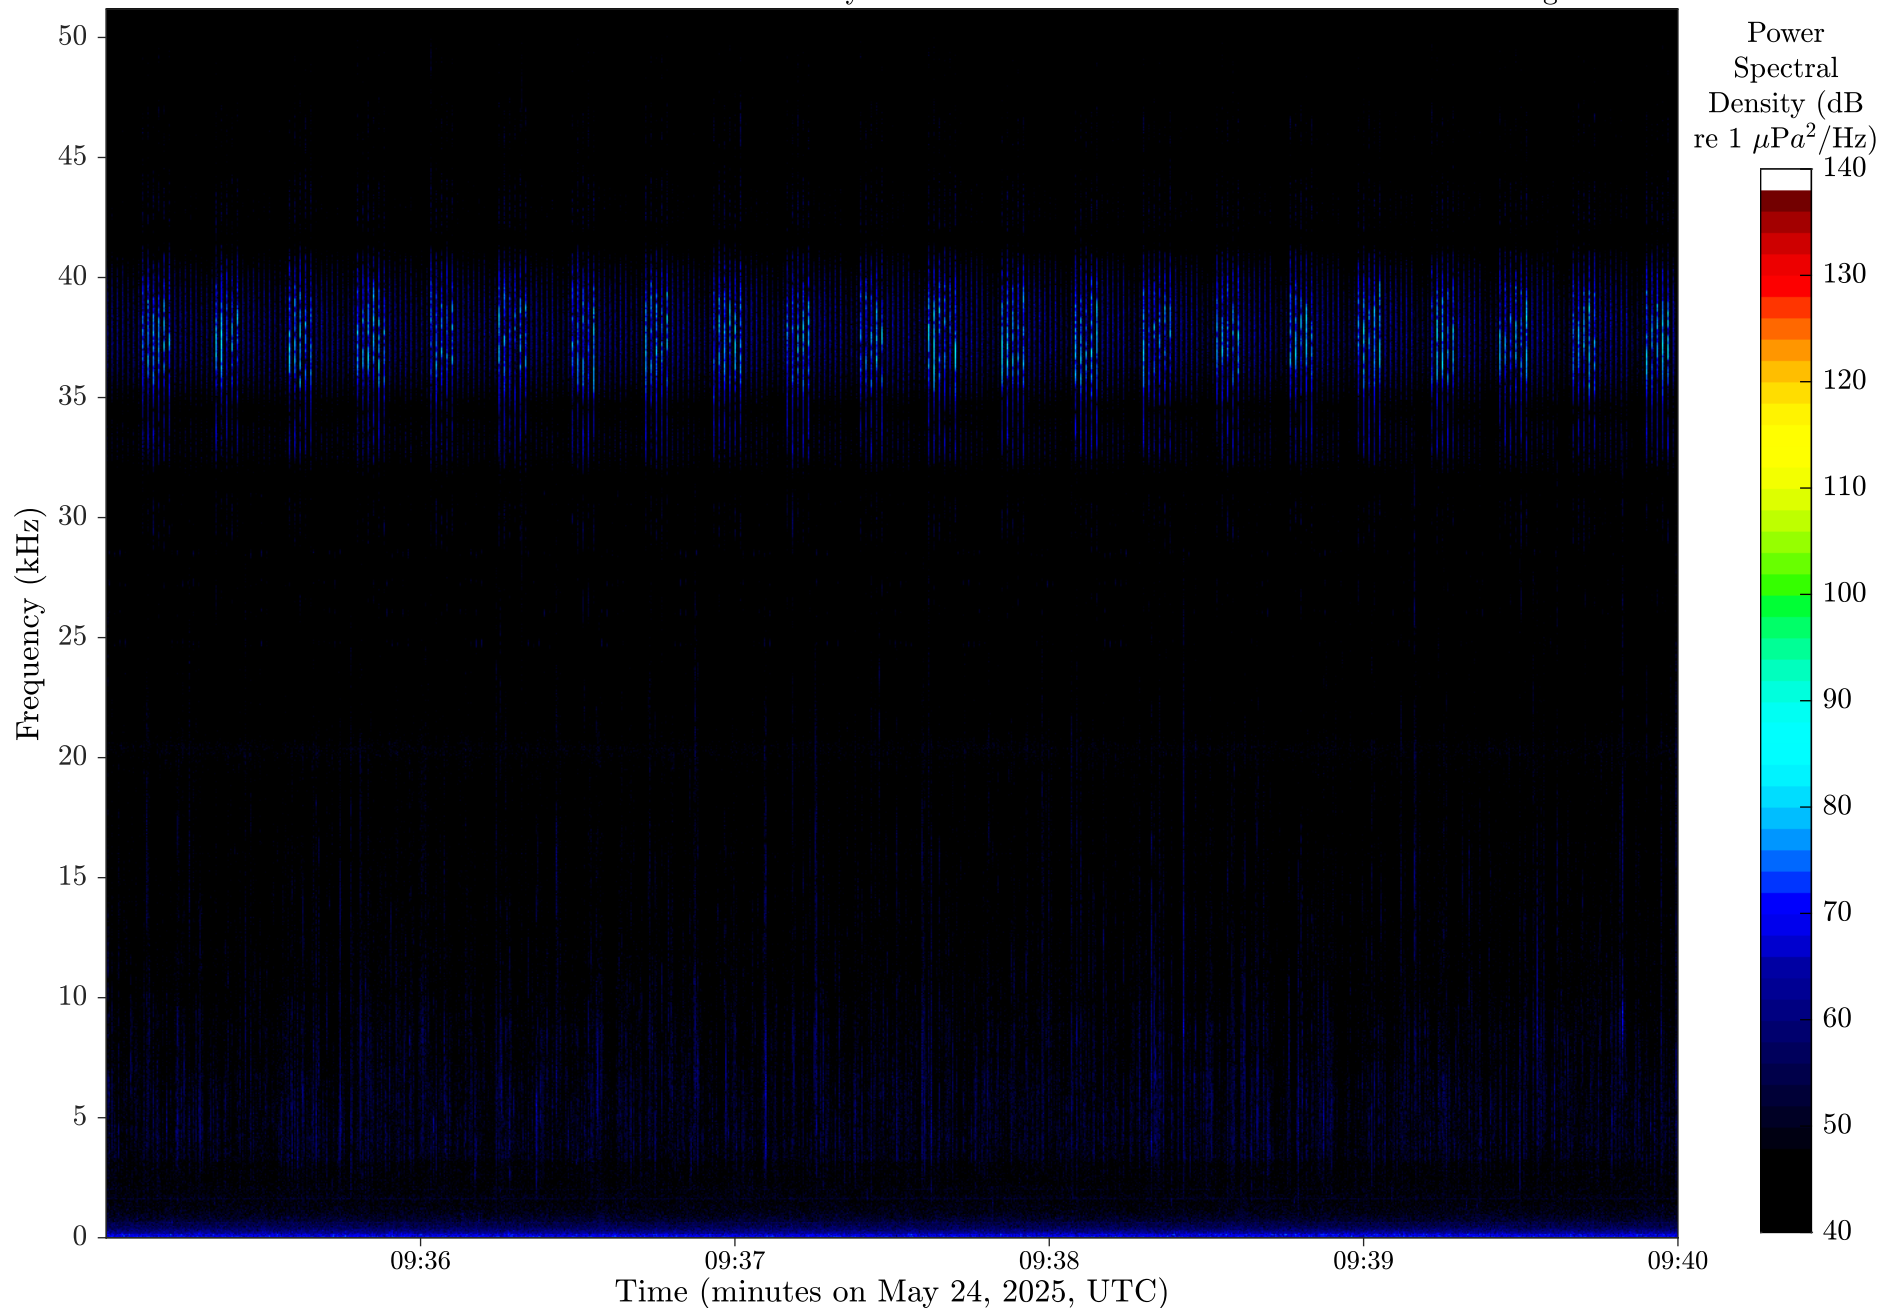

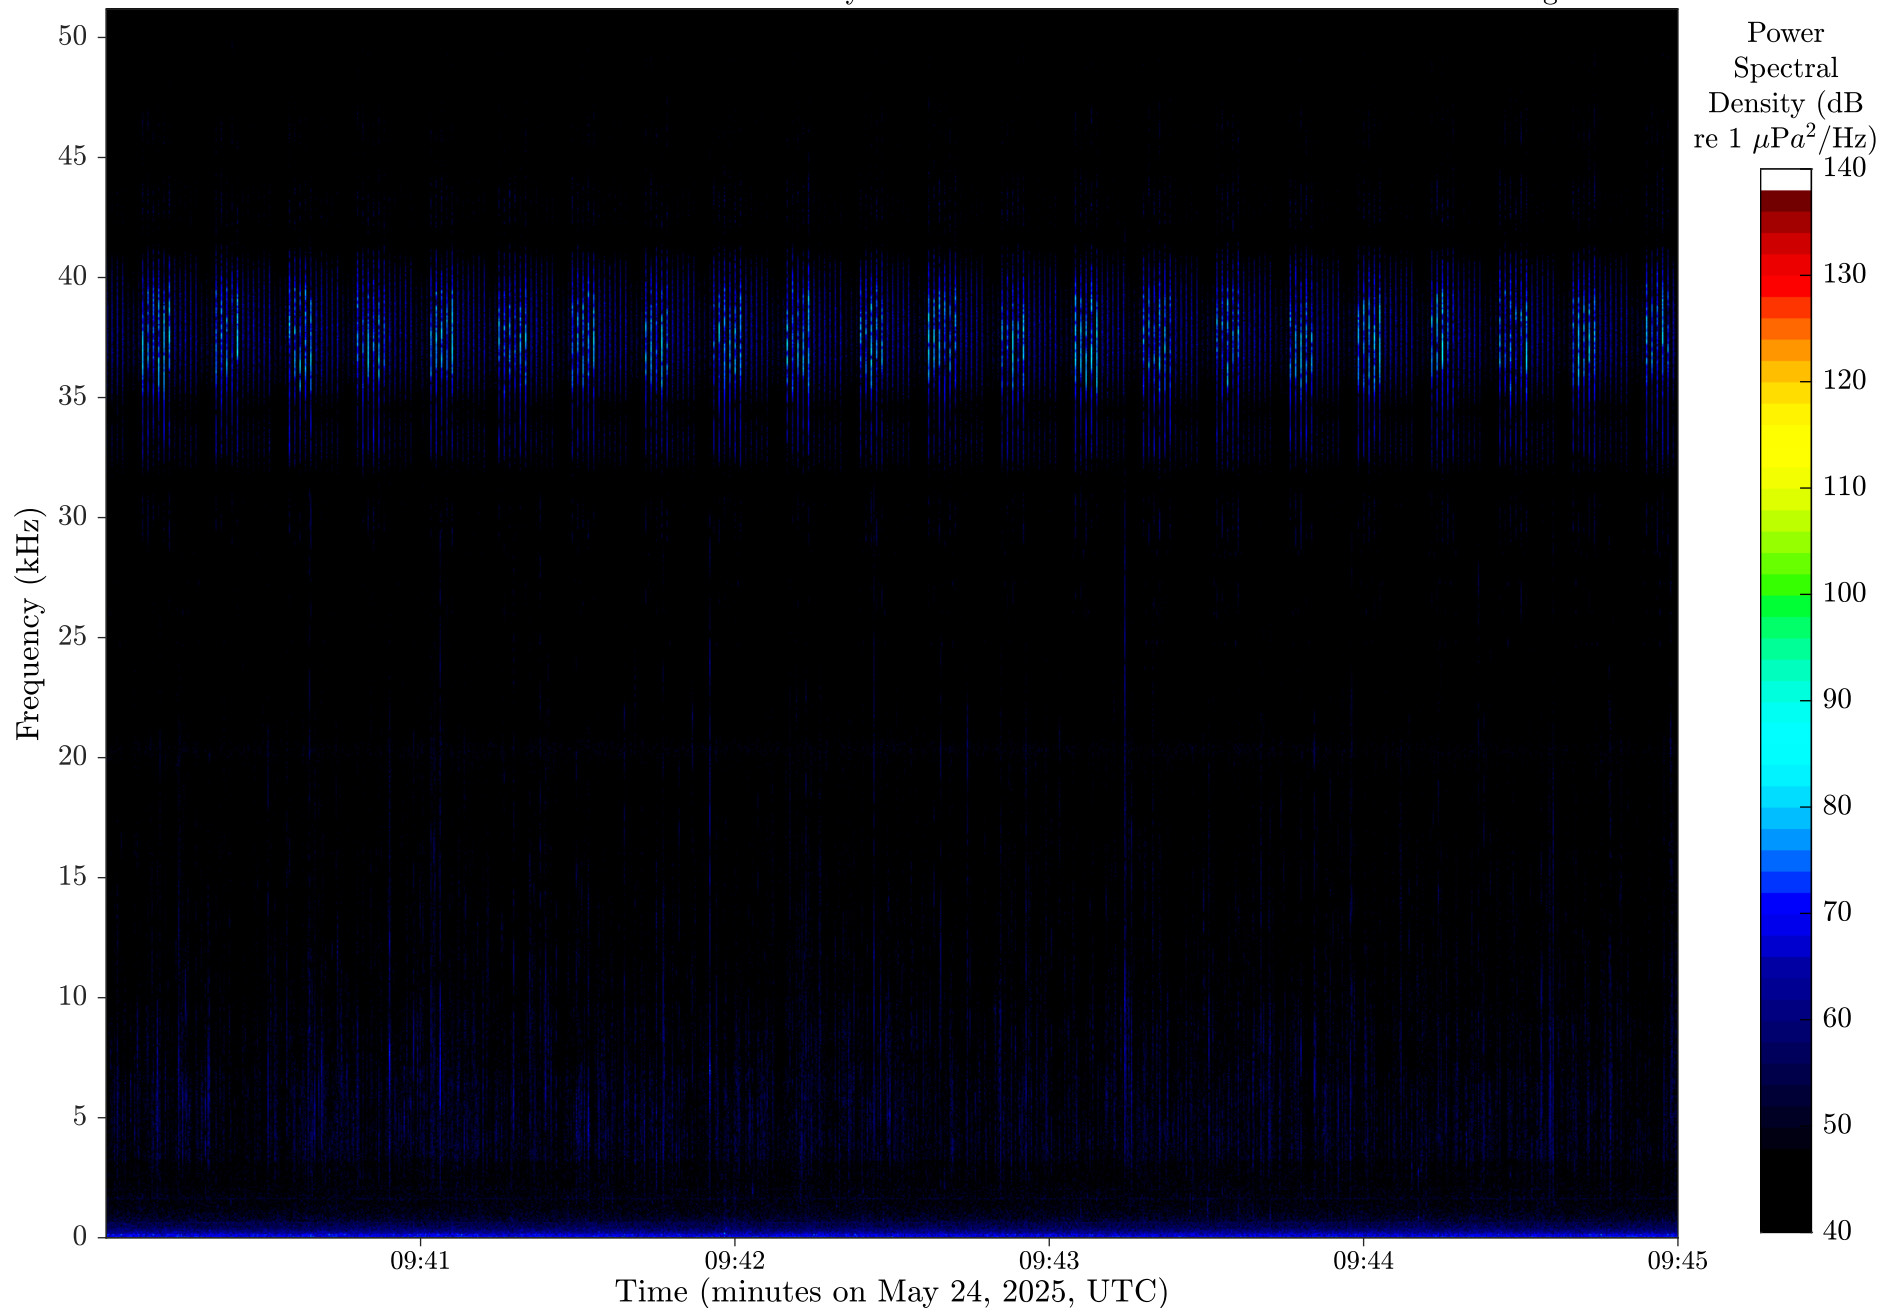


Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:08 UTC

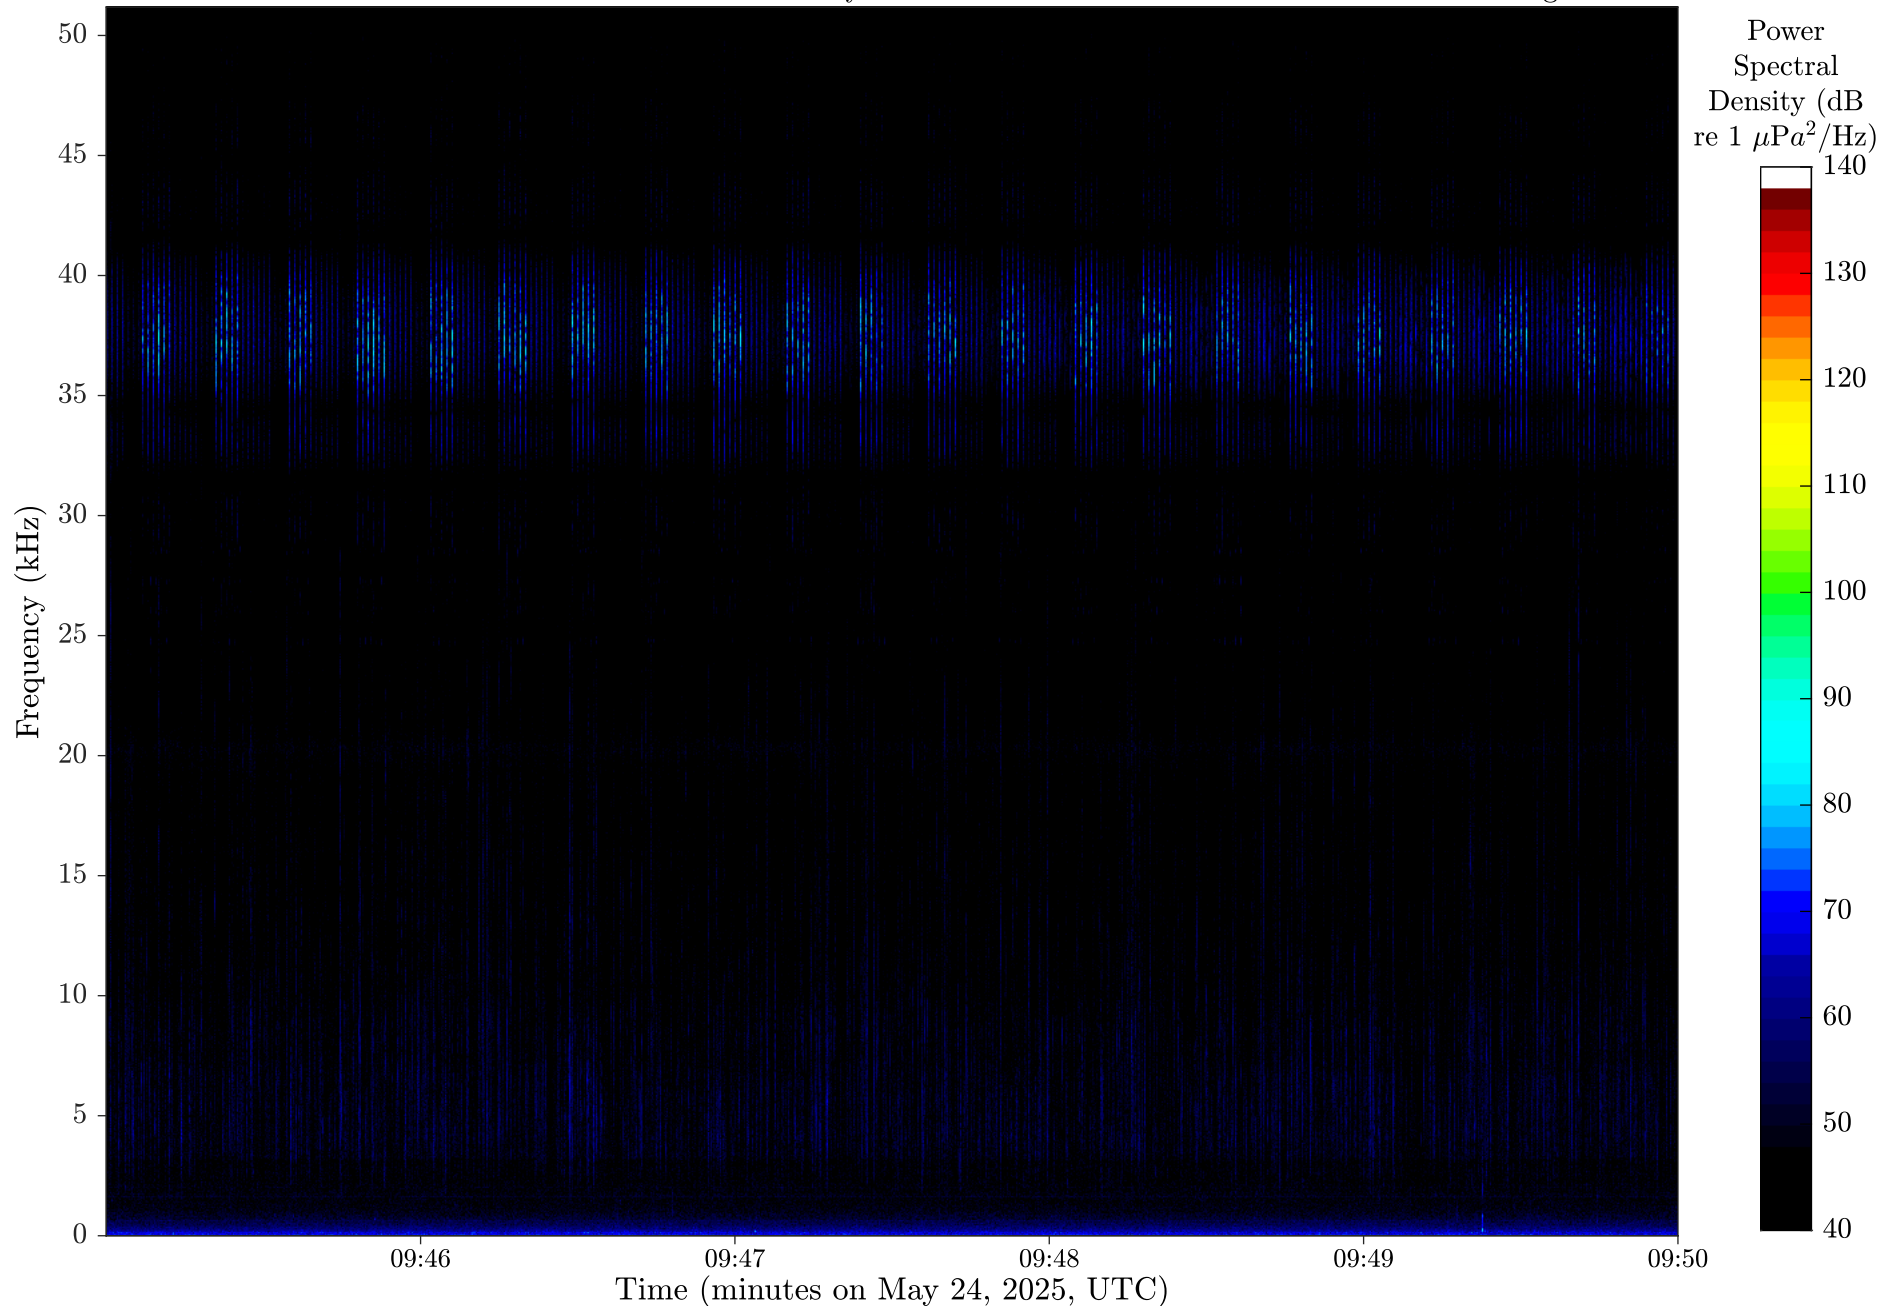


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:16 UTC

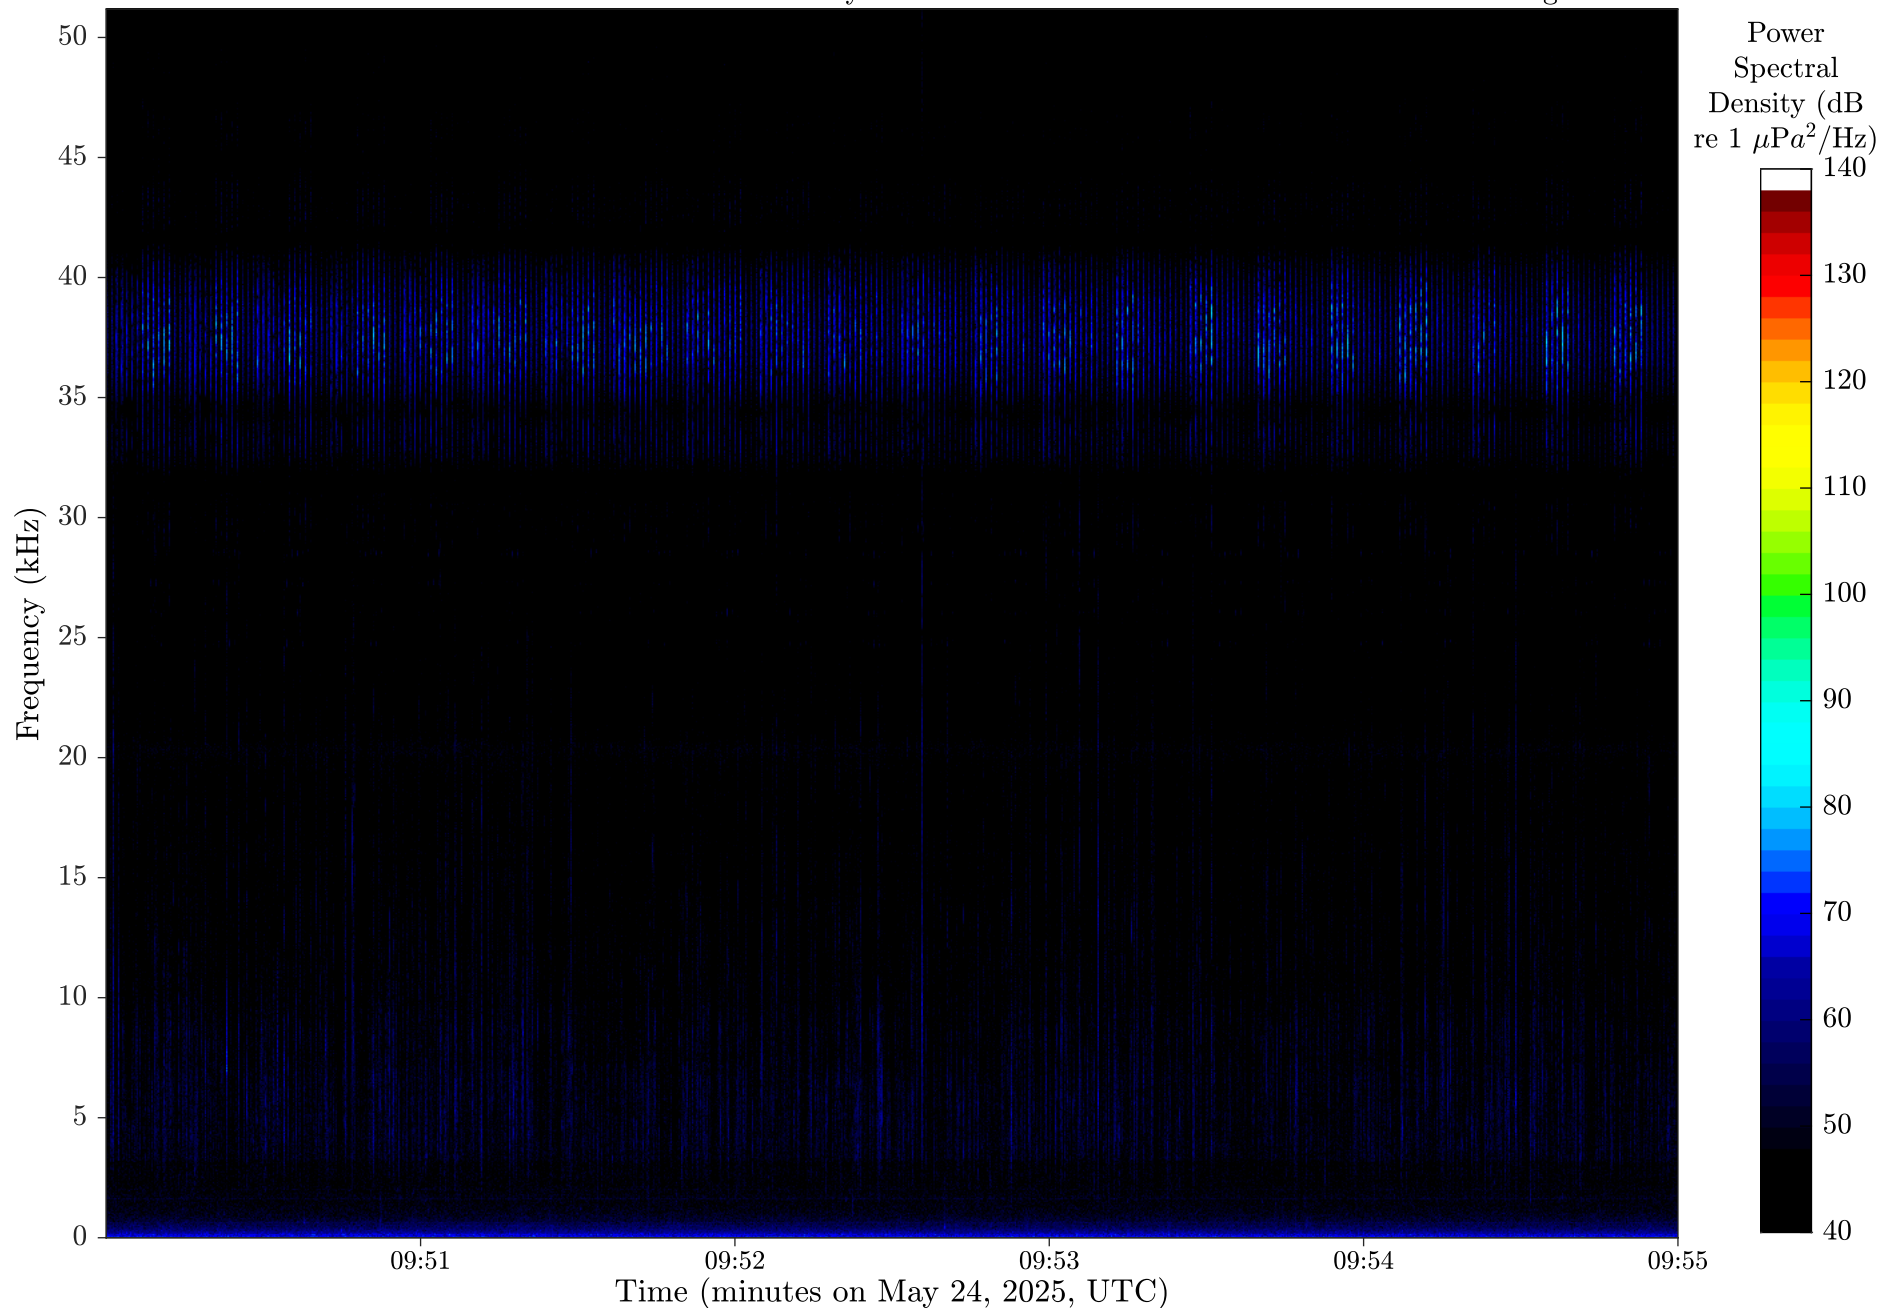


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:25 UTC

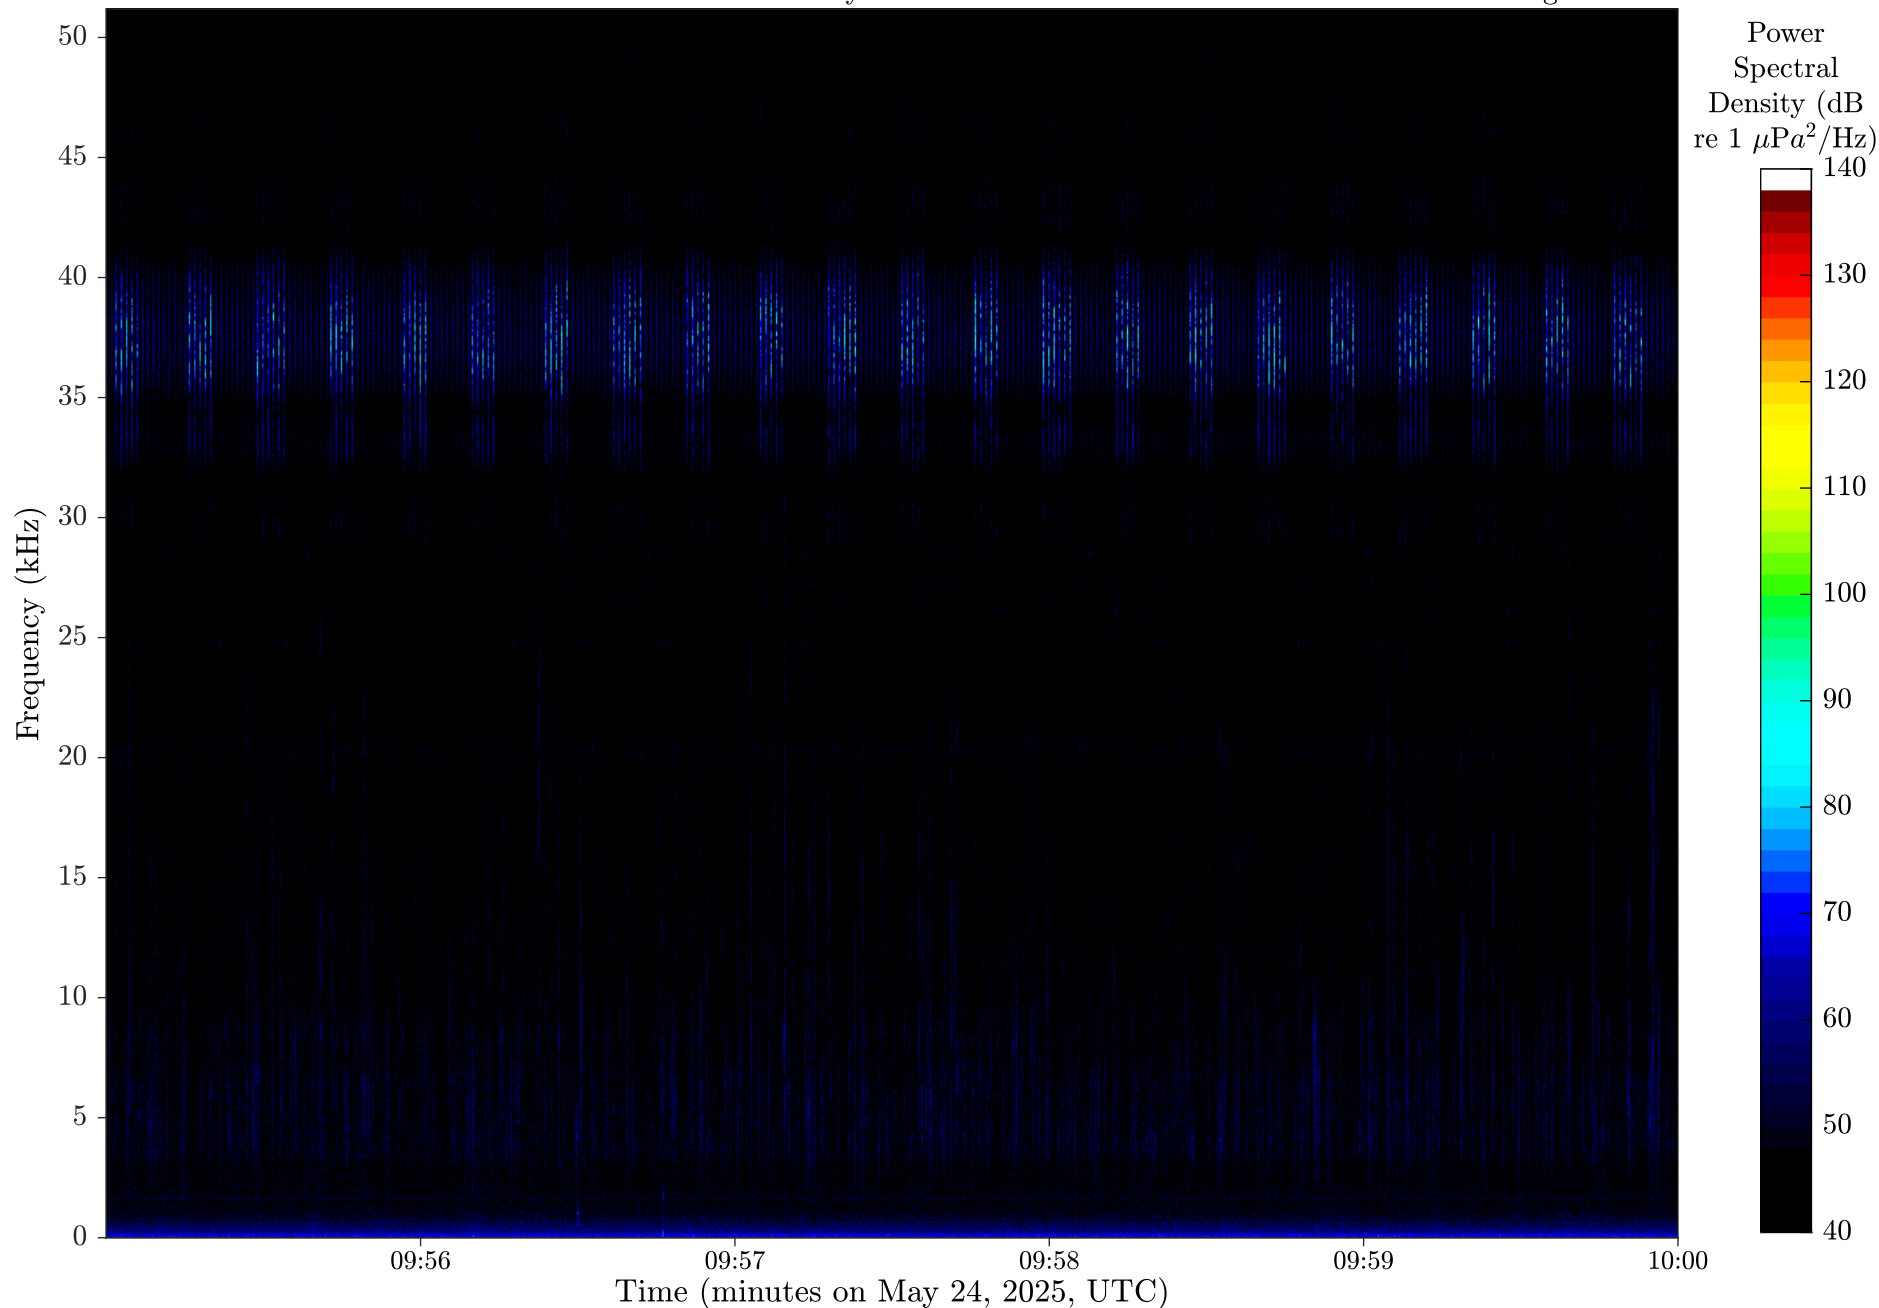


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:34 UTC

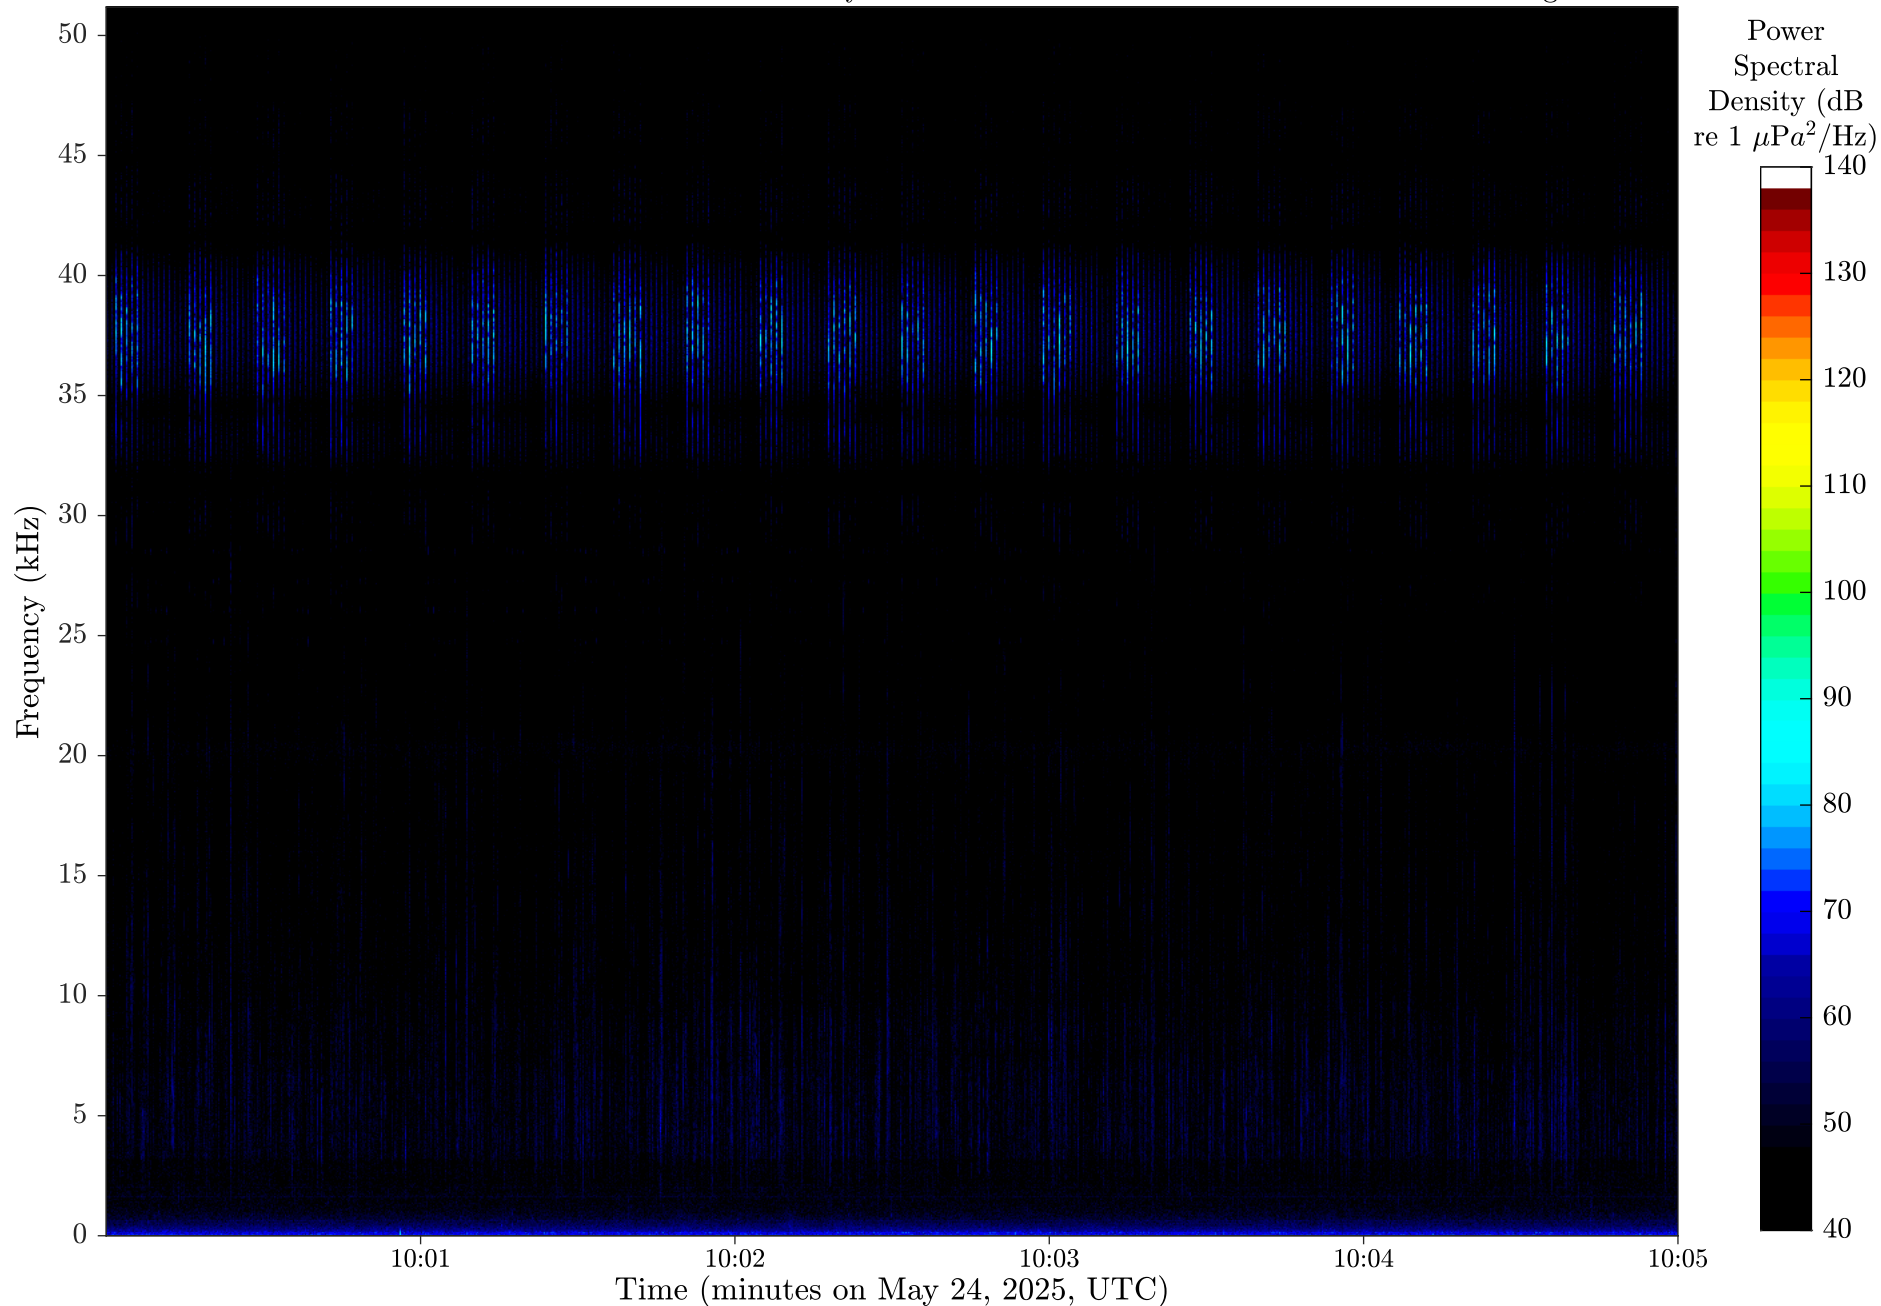


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:44 UTC

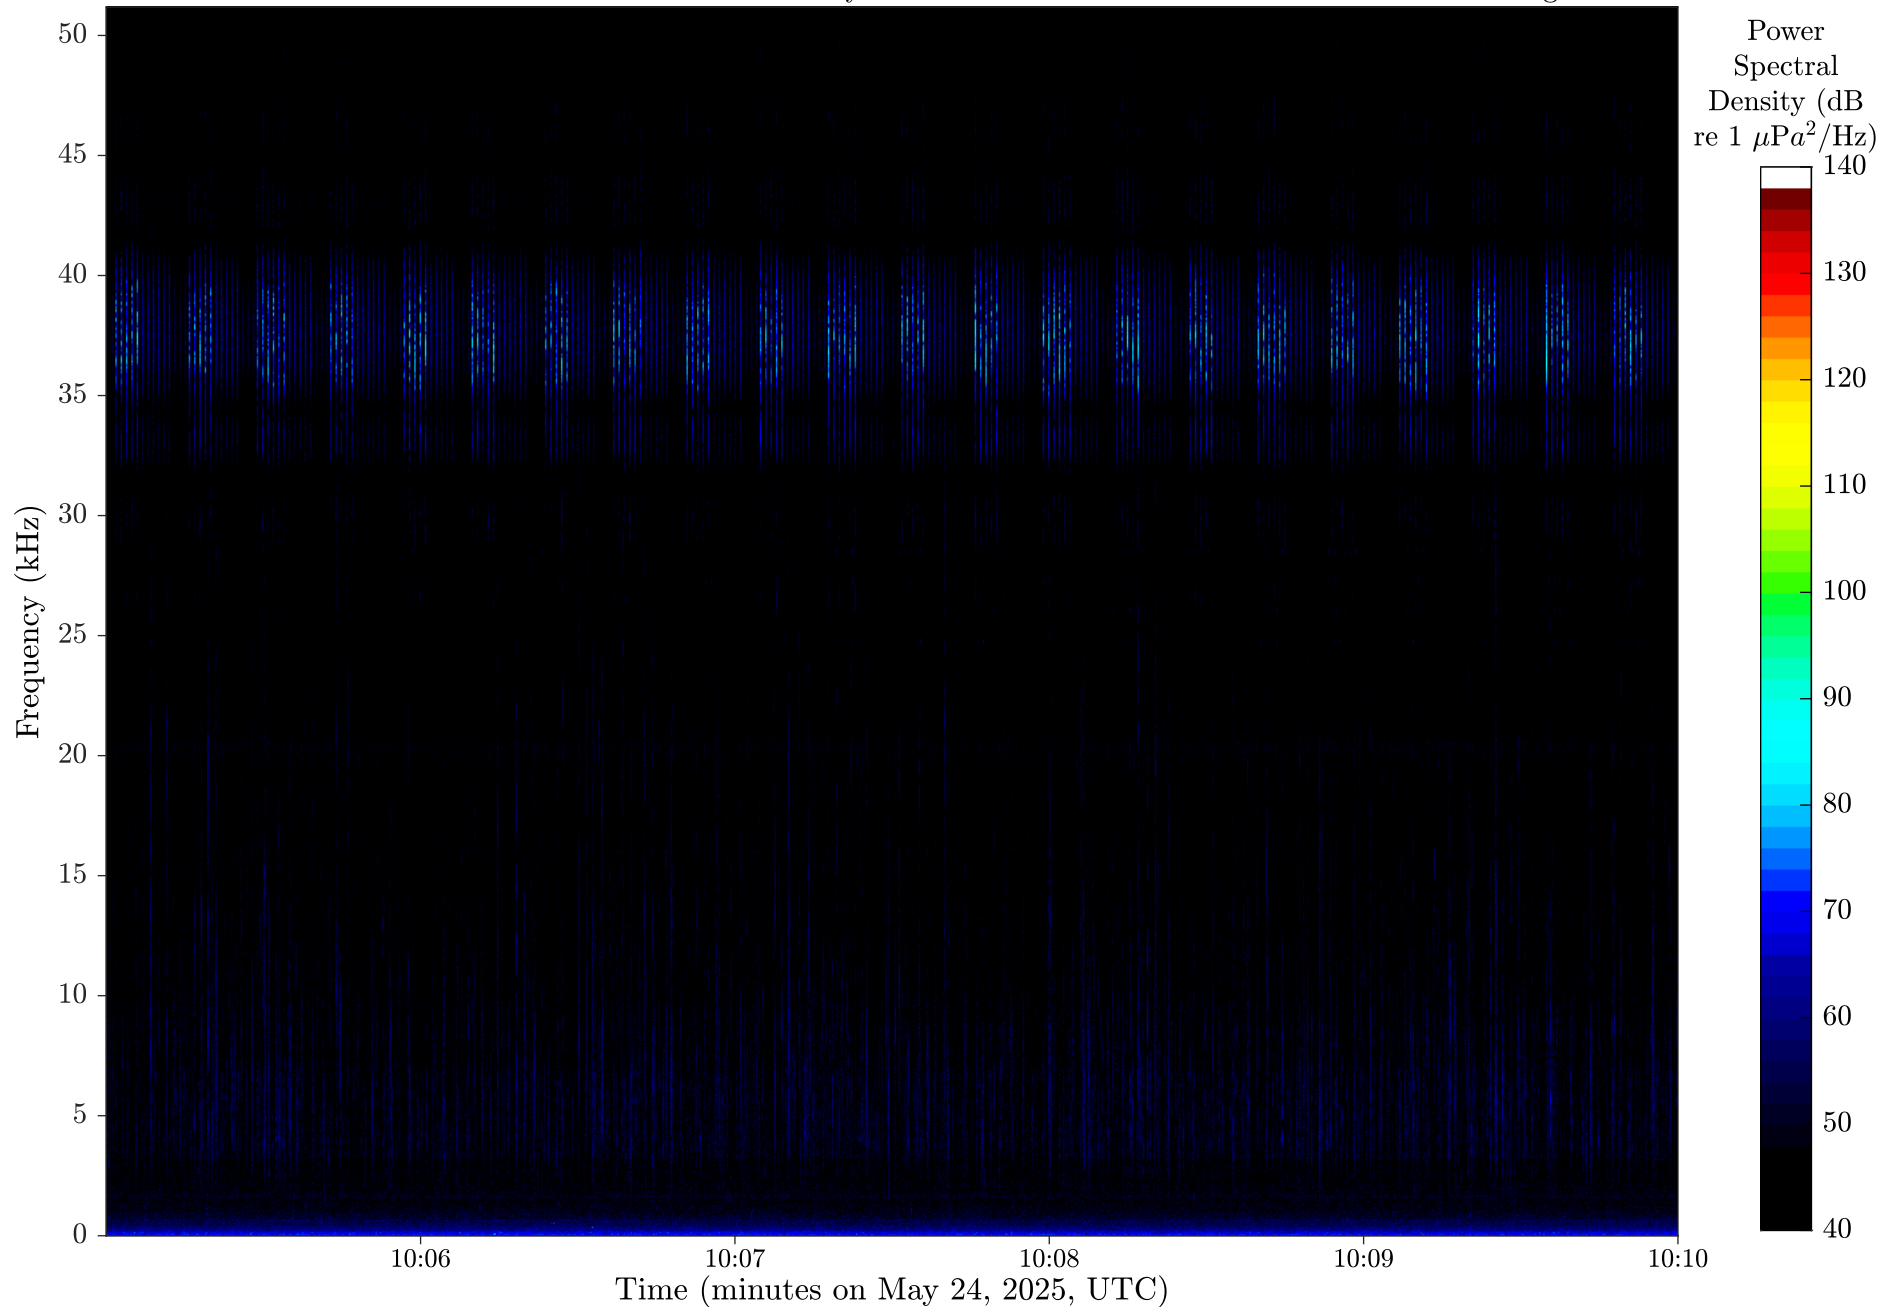


Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:31:52 UTC

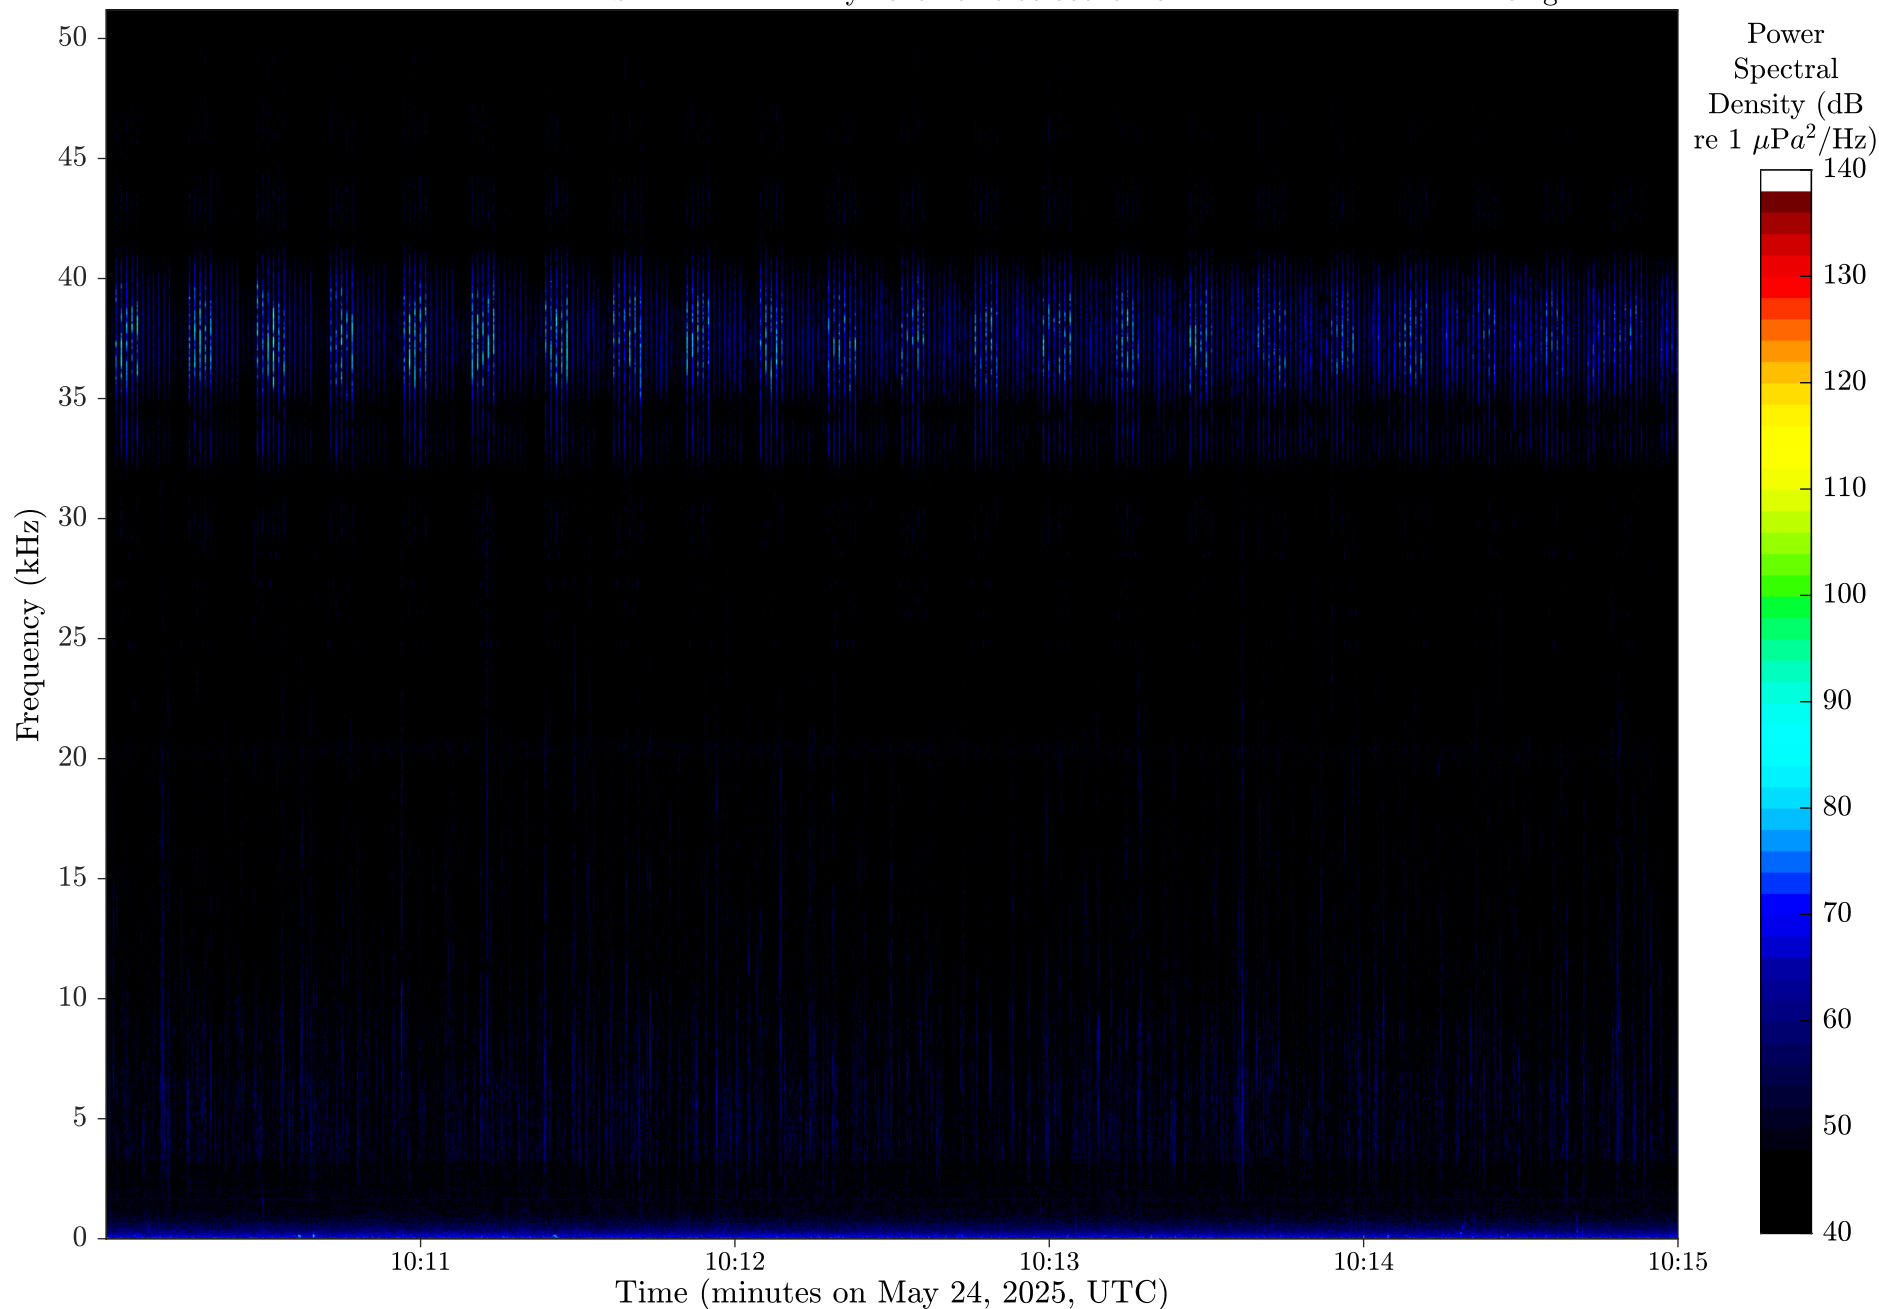


Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:32:01 UTC

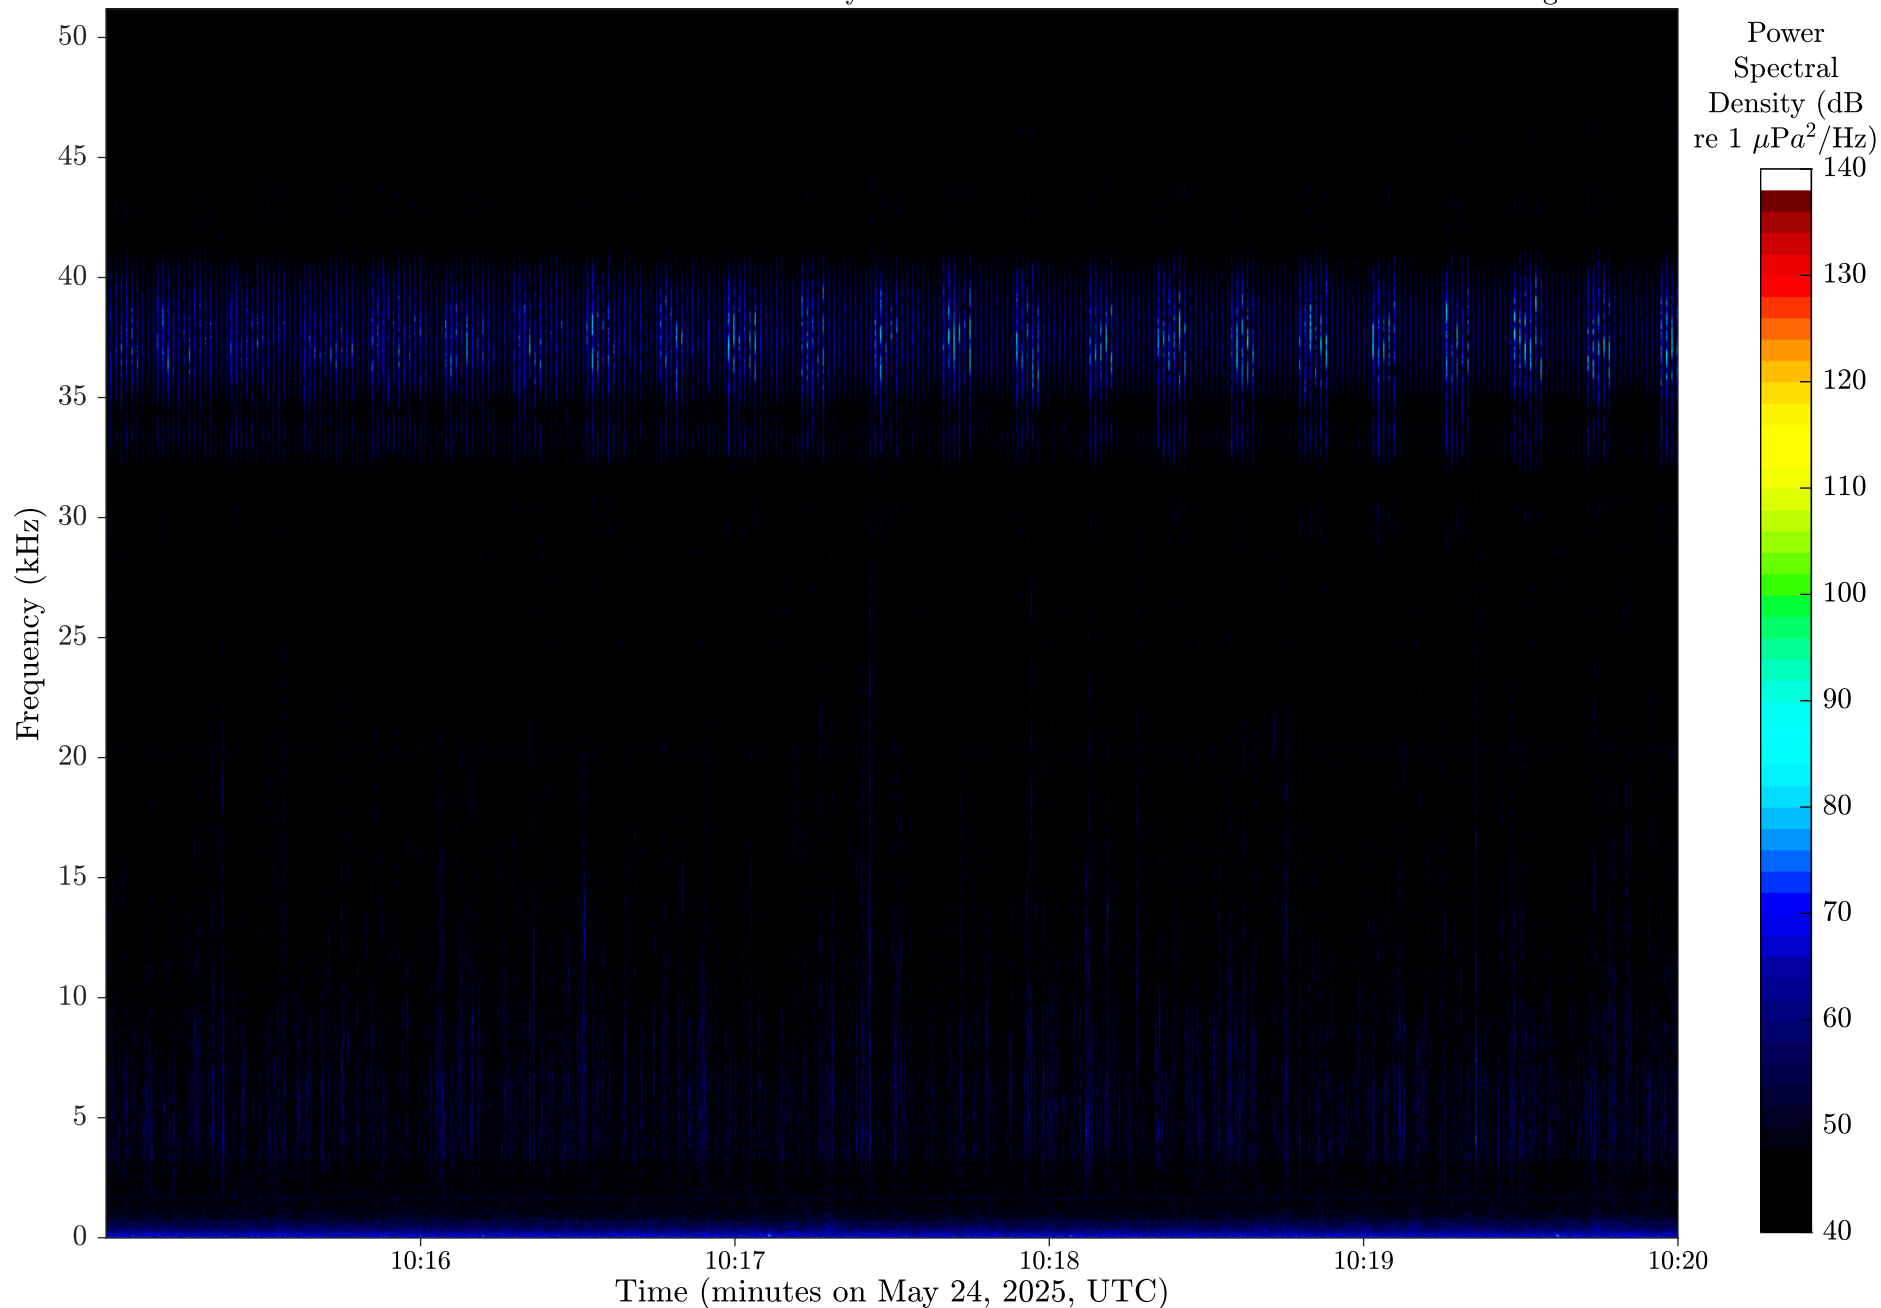


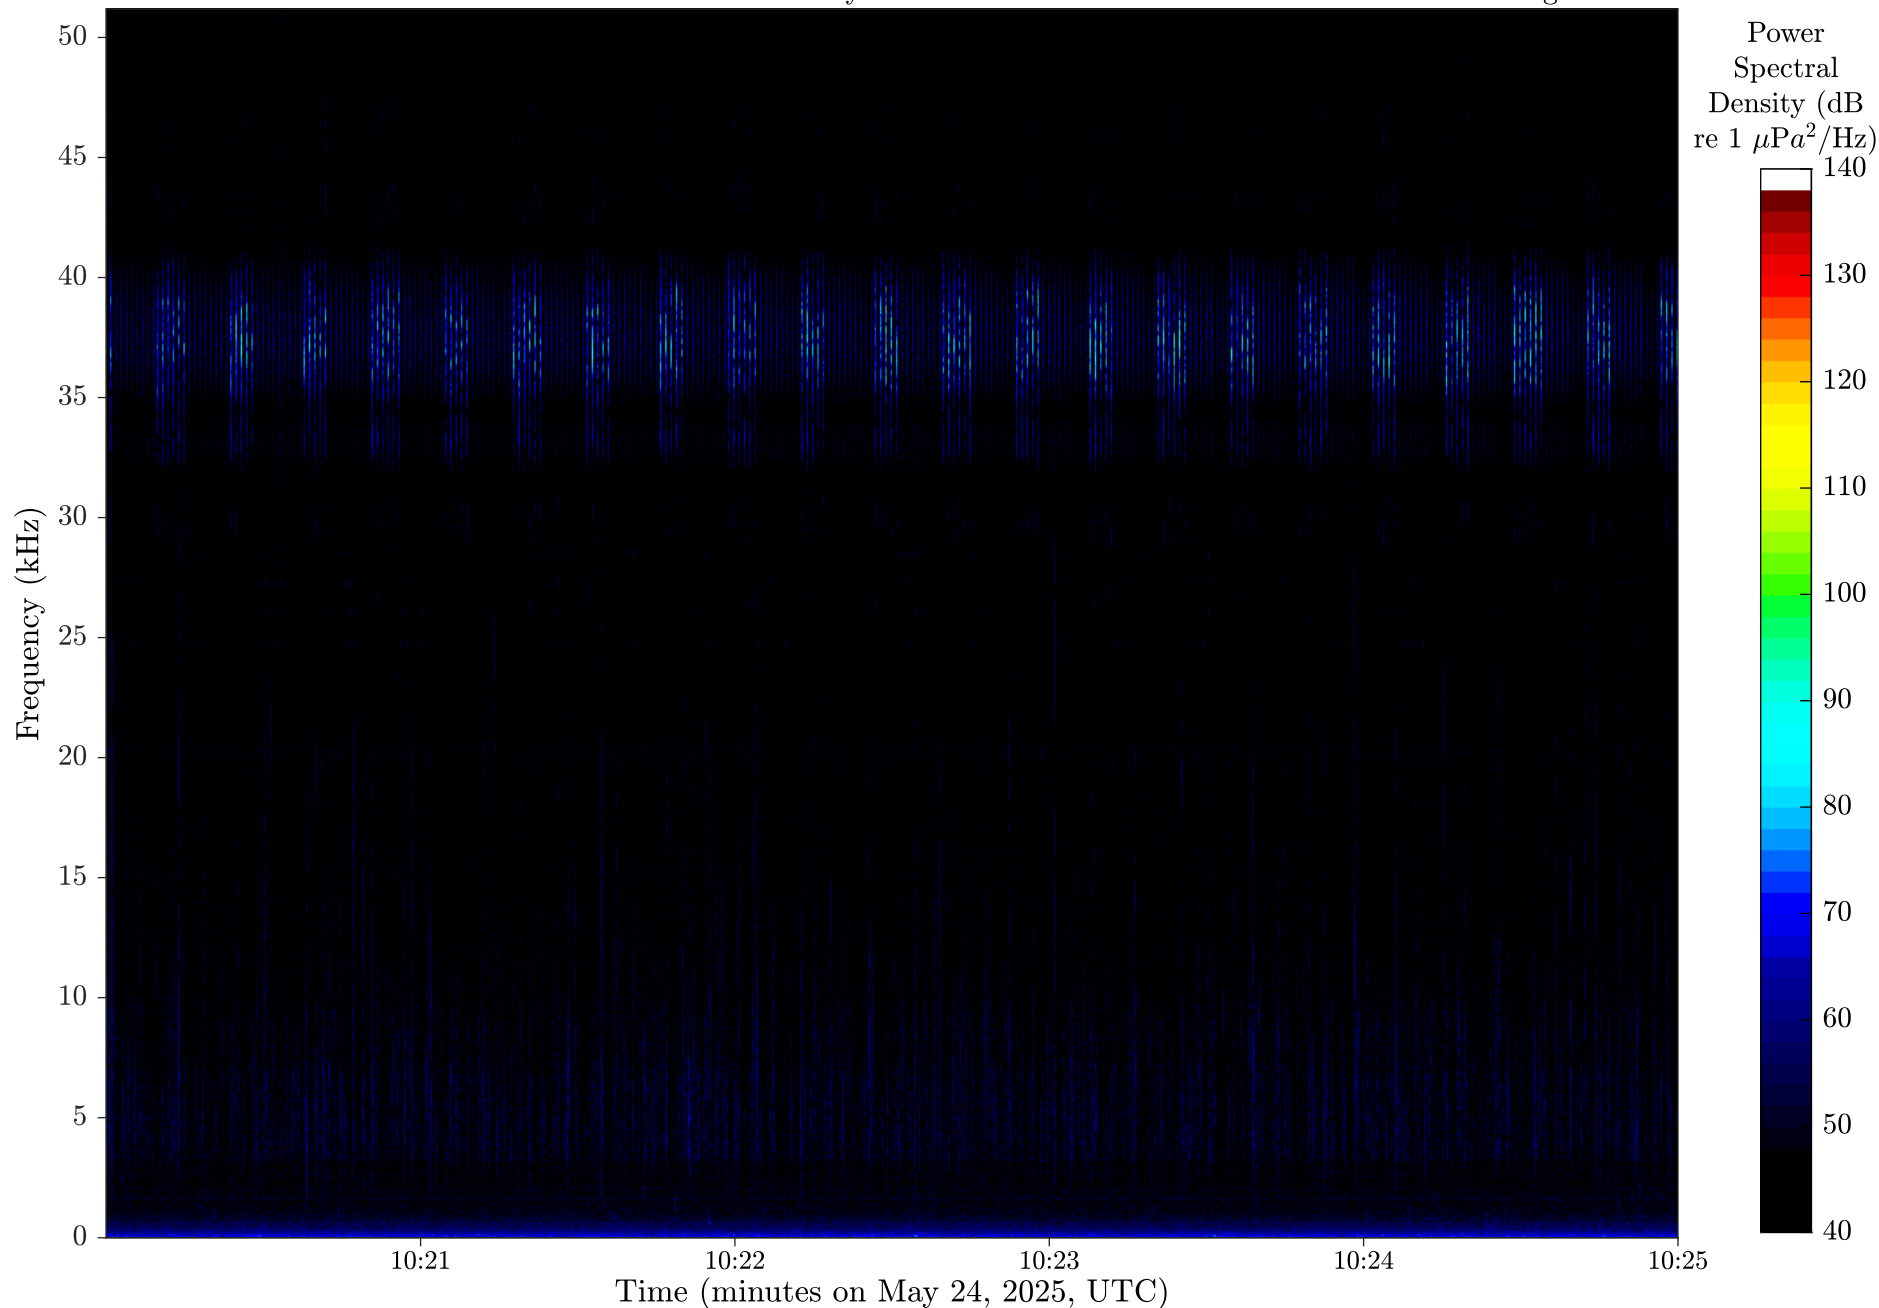

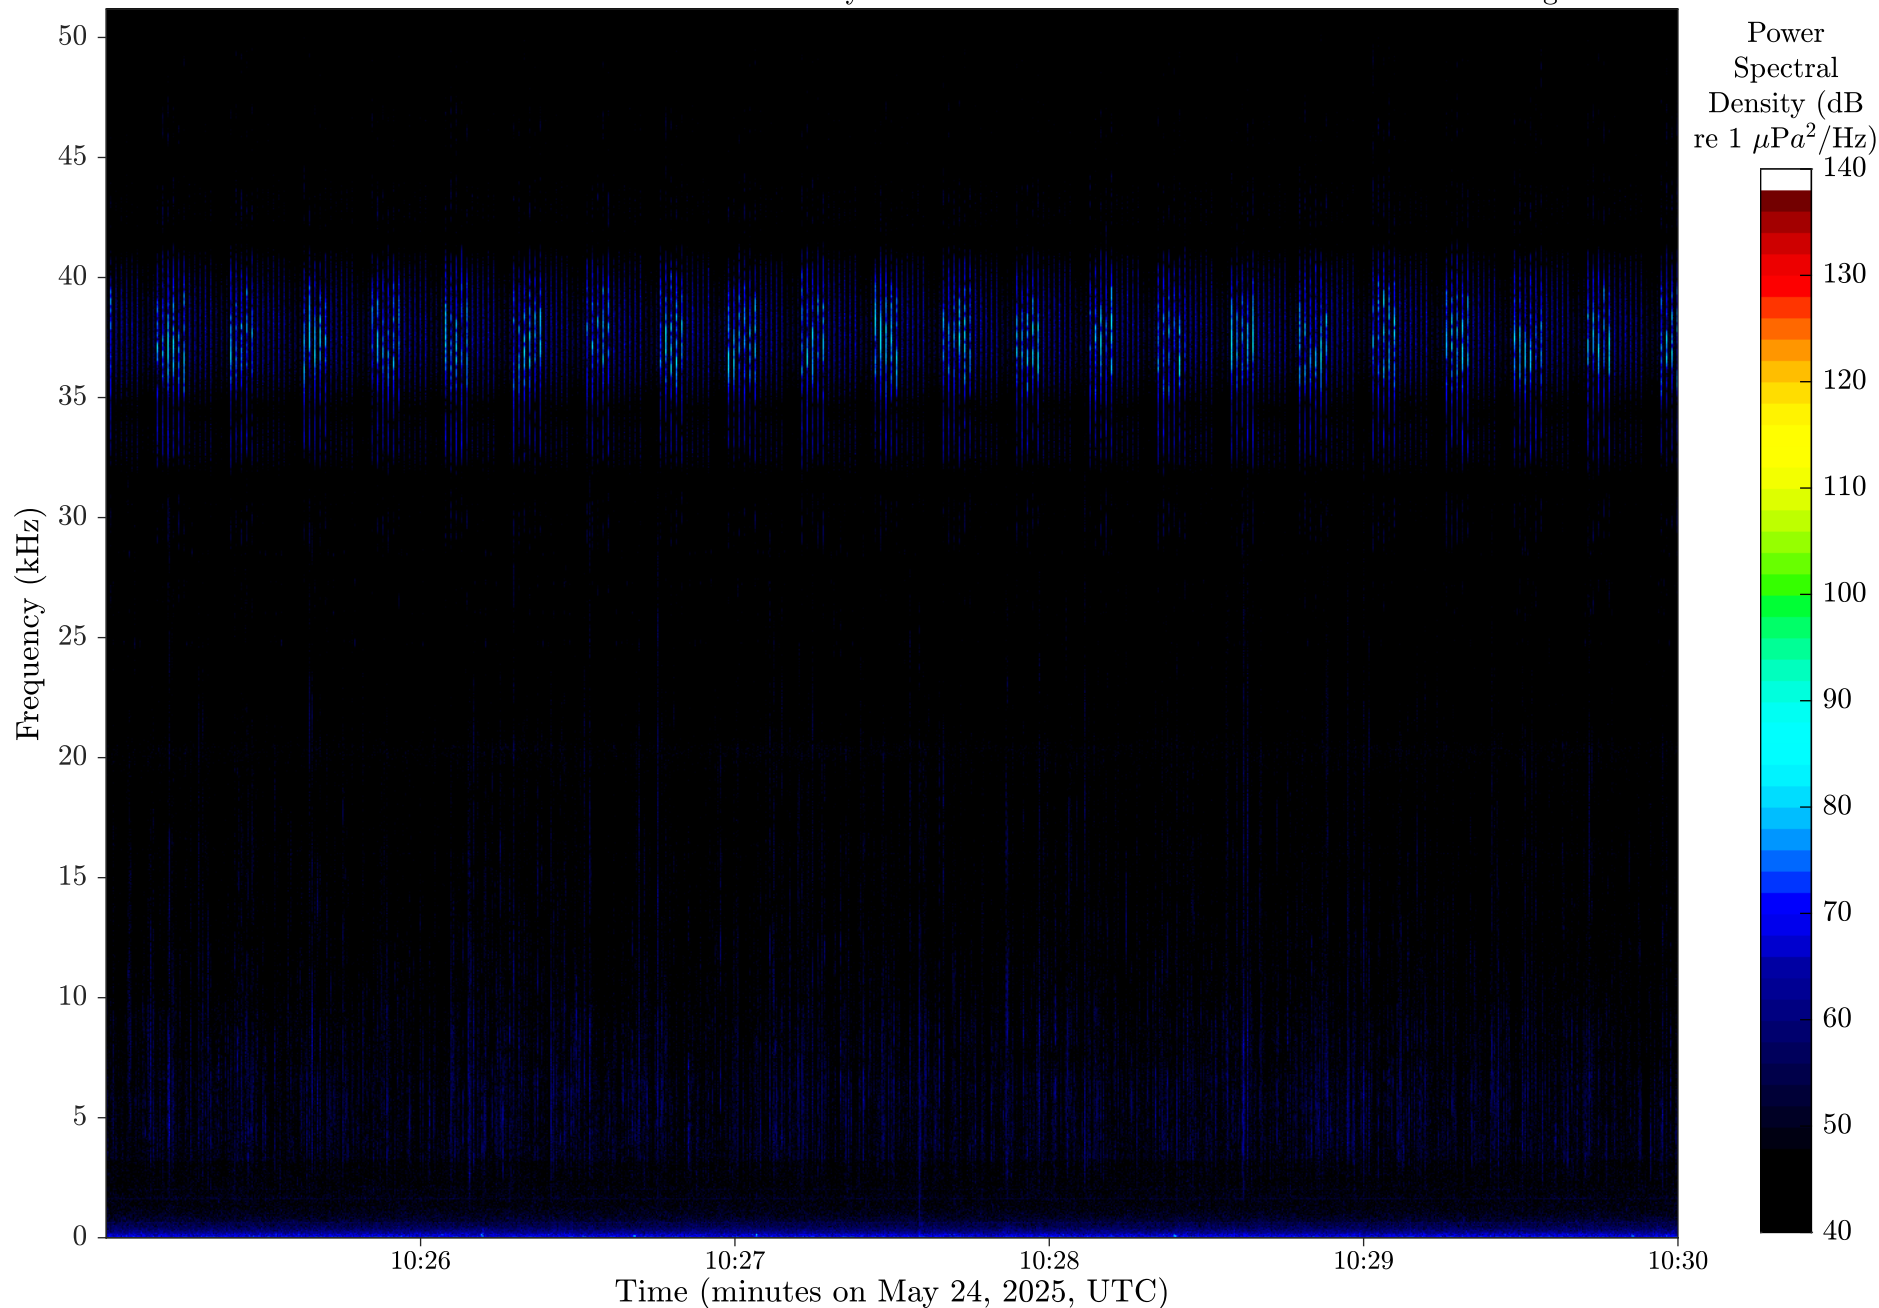


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:32:28 UTC

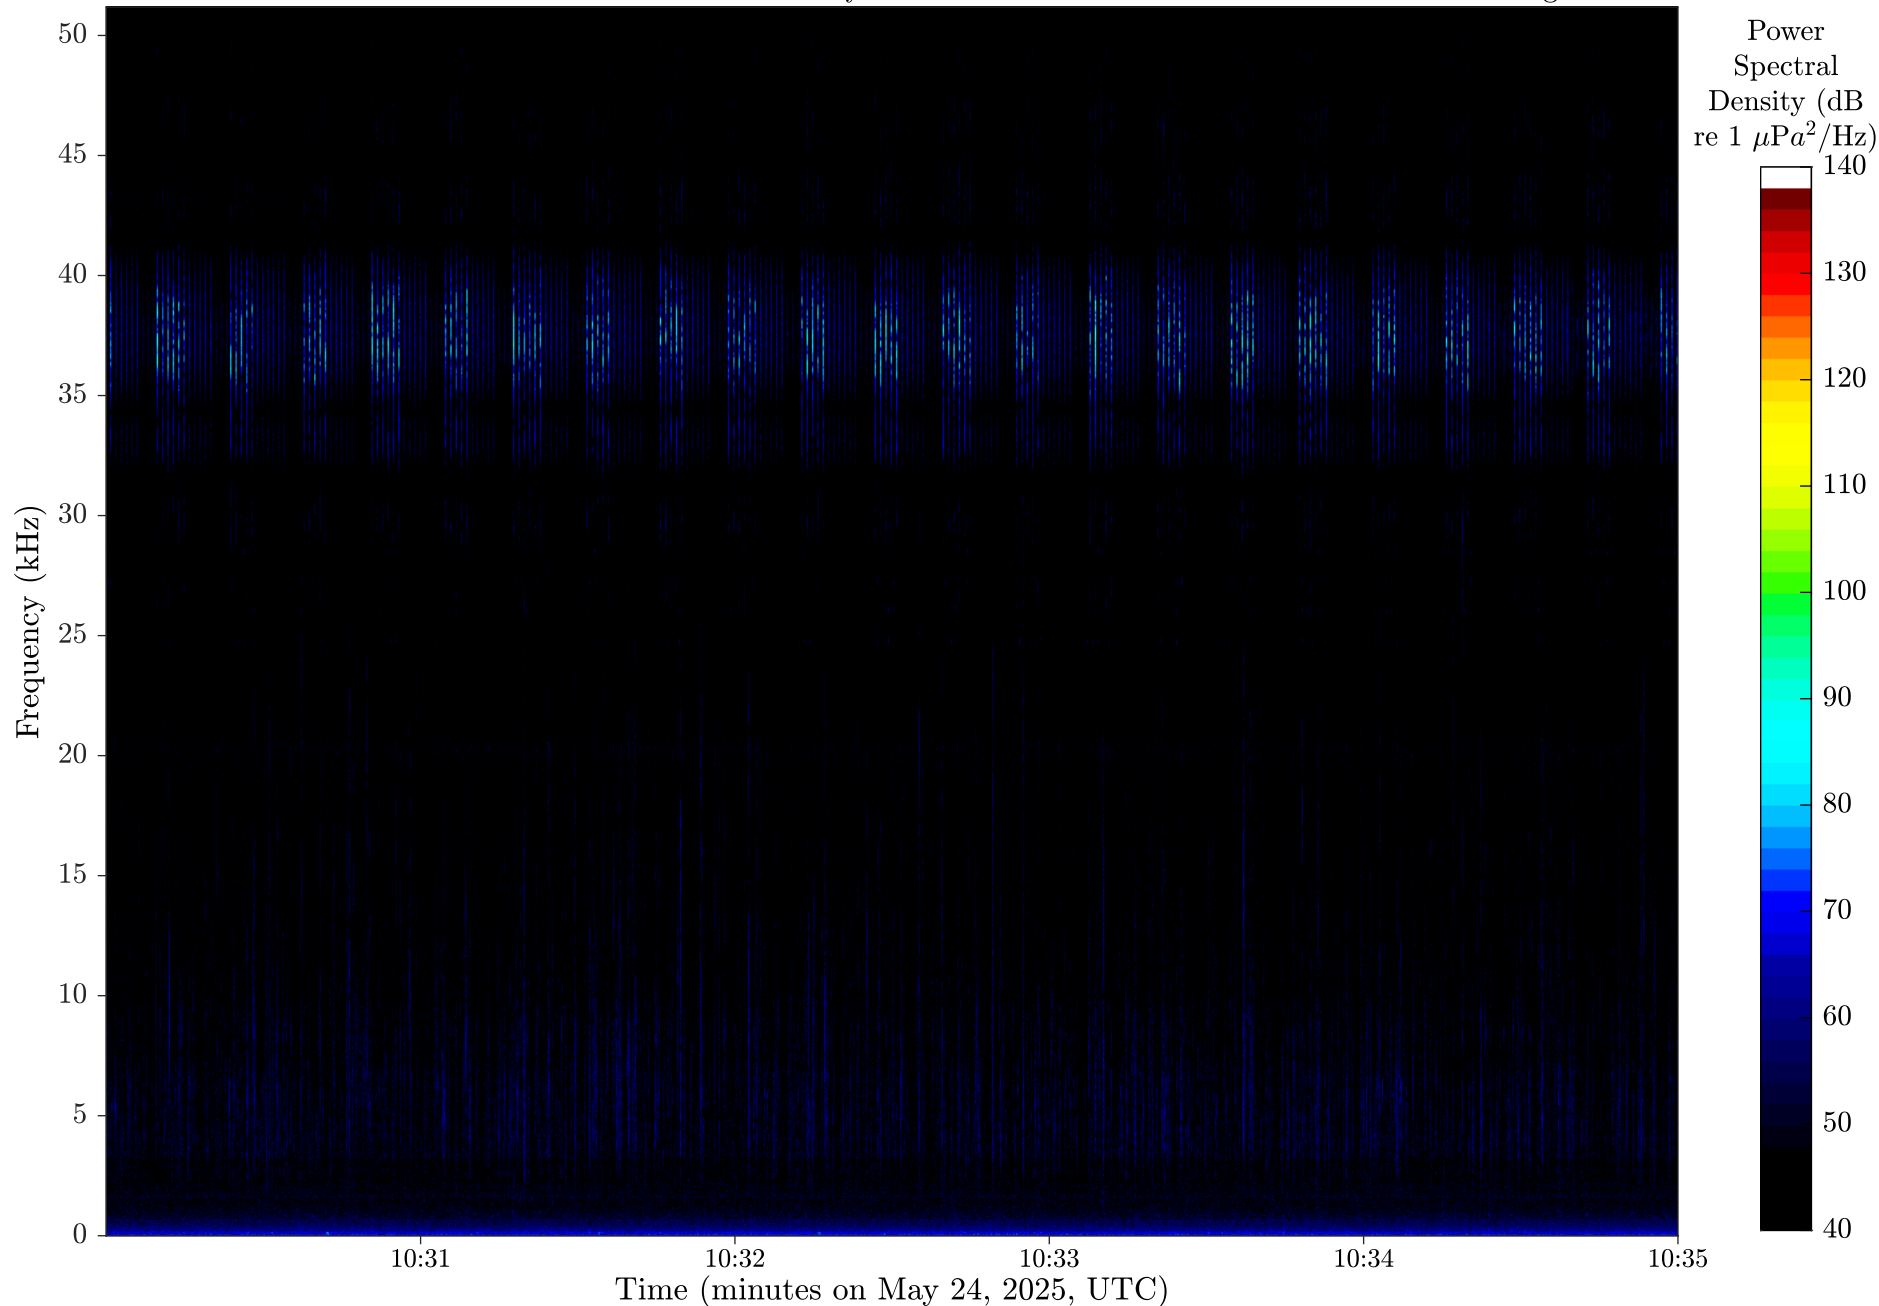


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:32:36 UTC

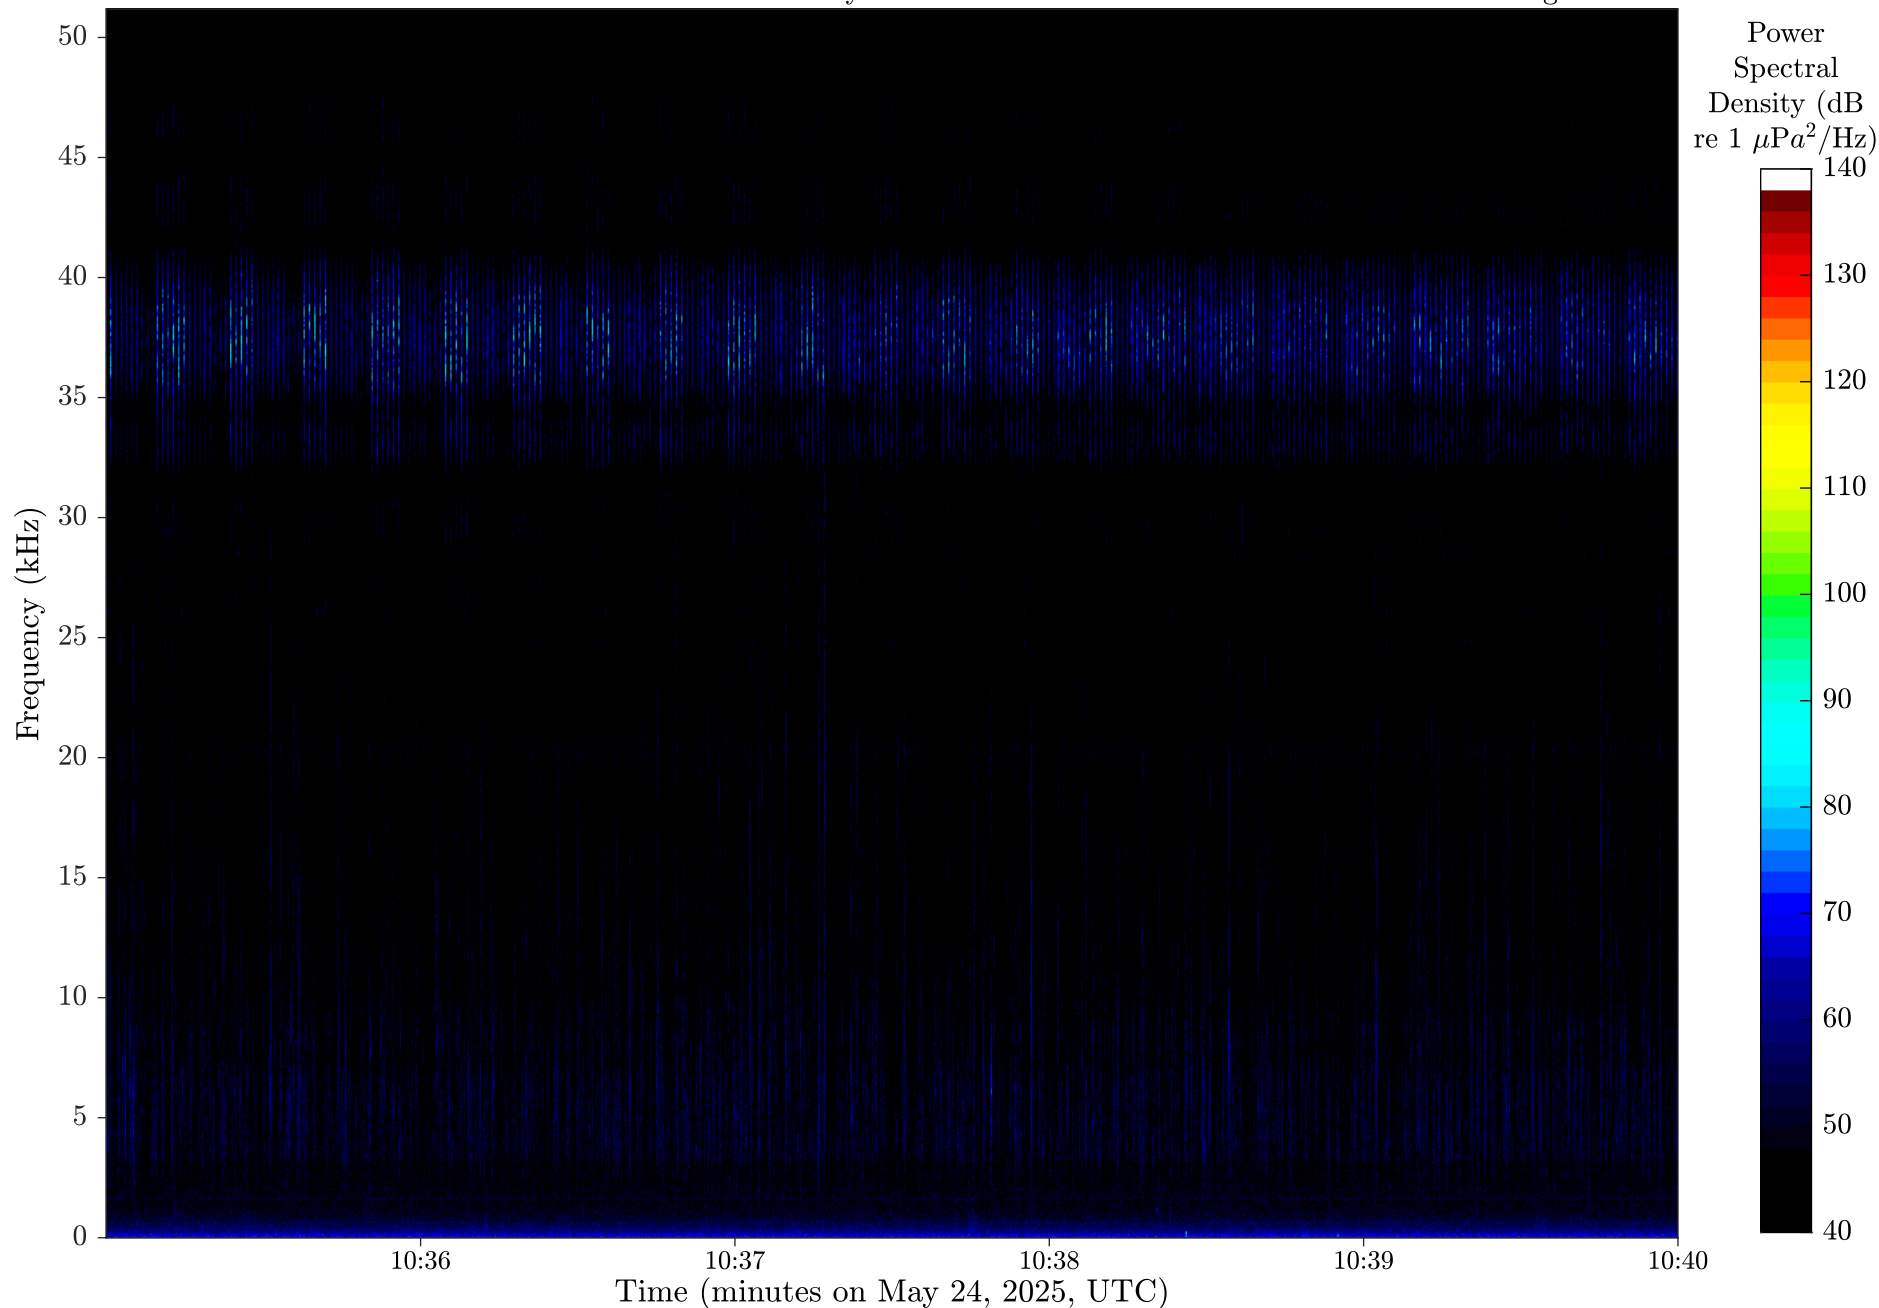


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:32:44 UTC

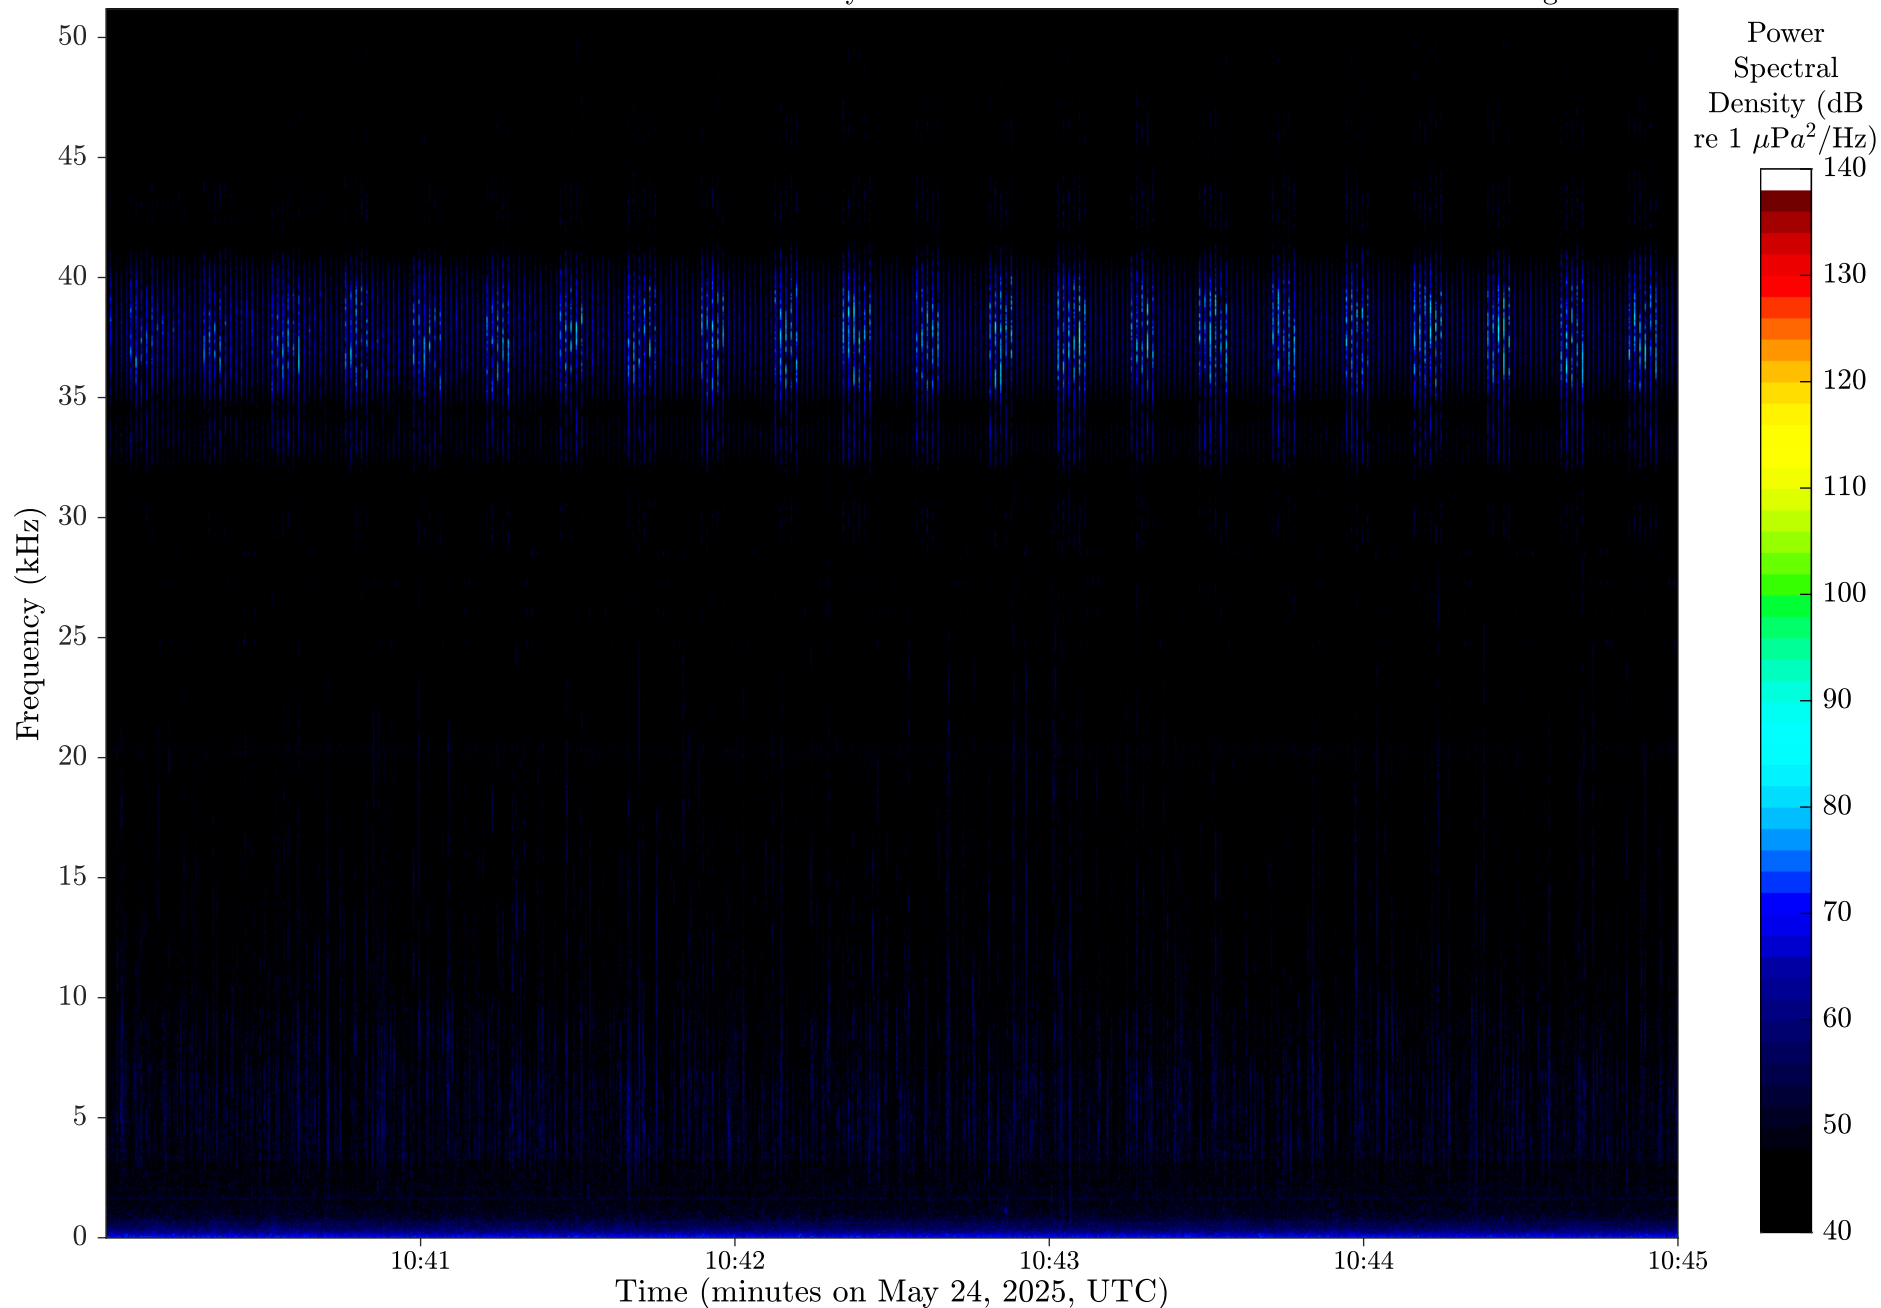


Comments: 33.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:32:53 UTC

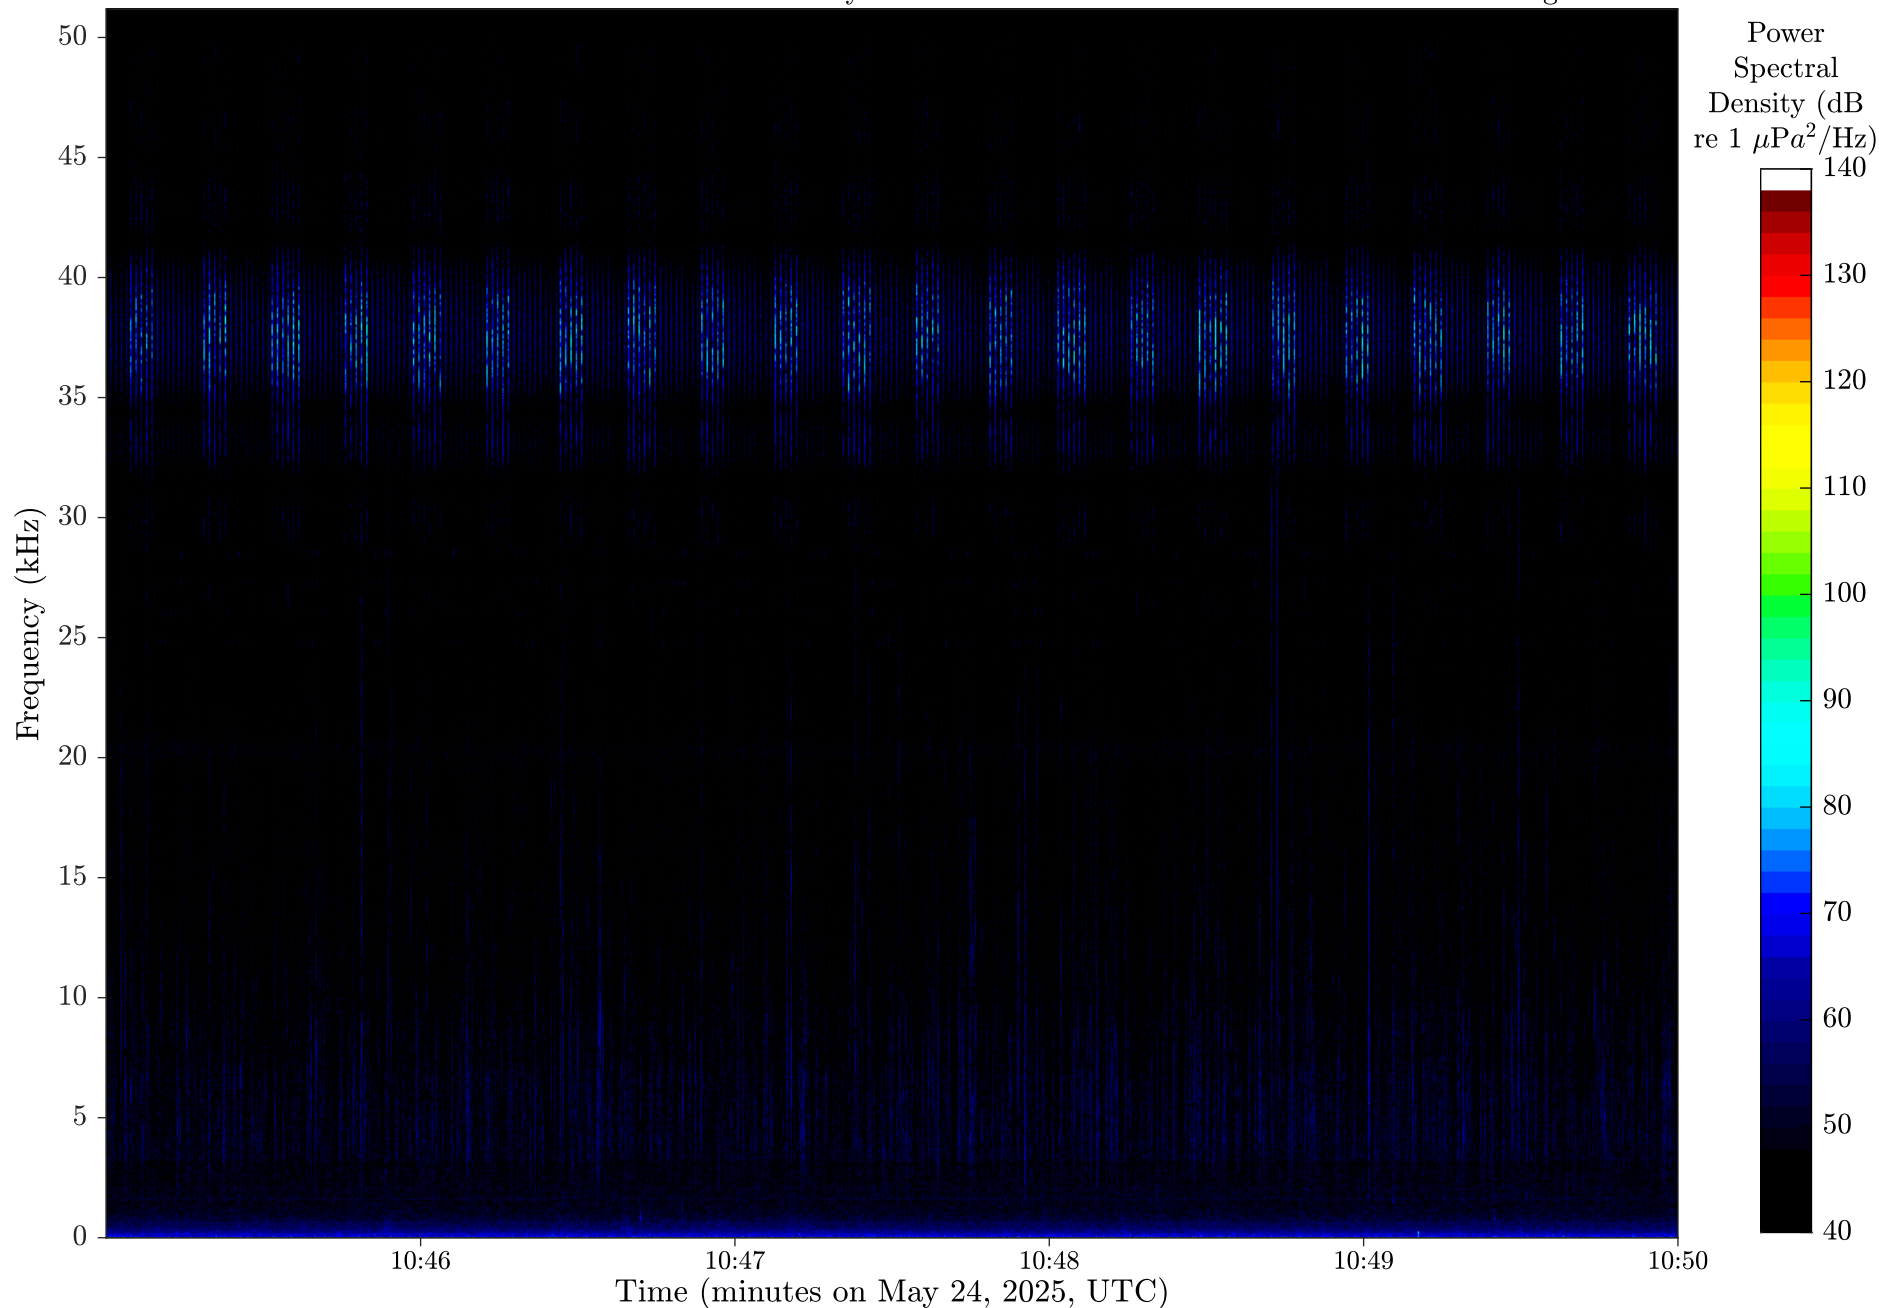


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:33:02 UTC

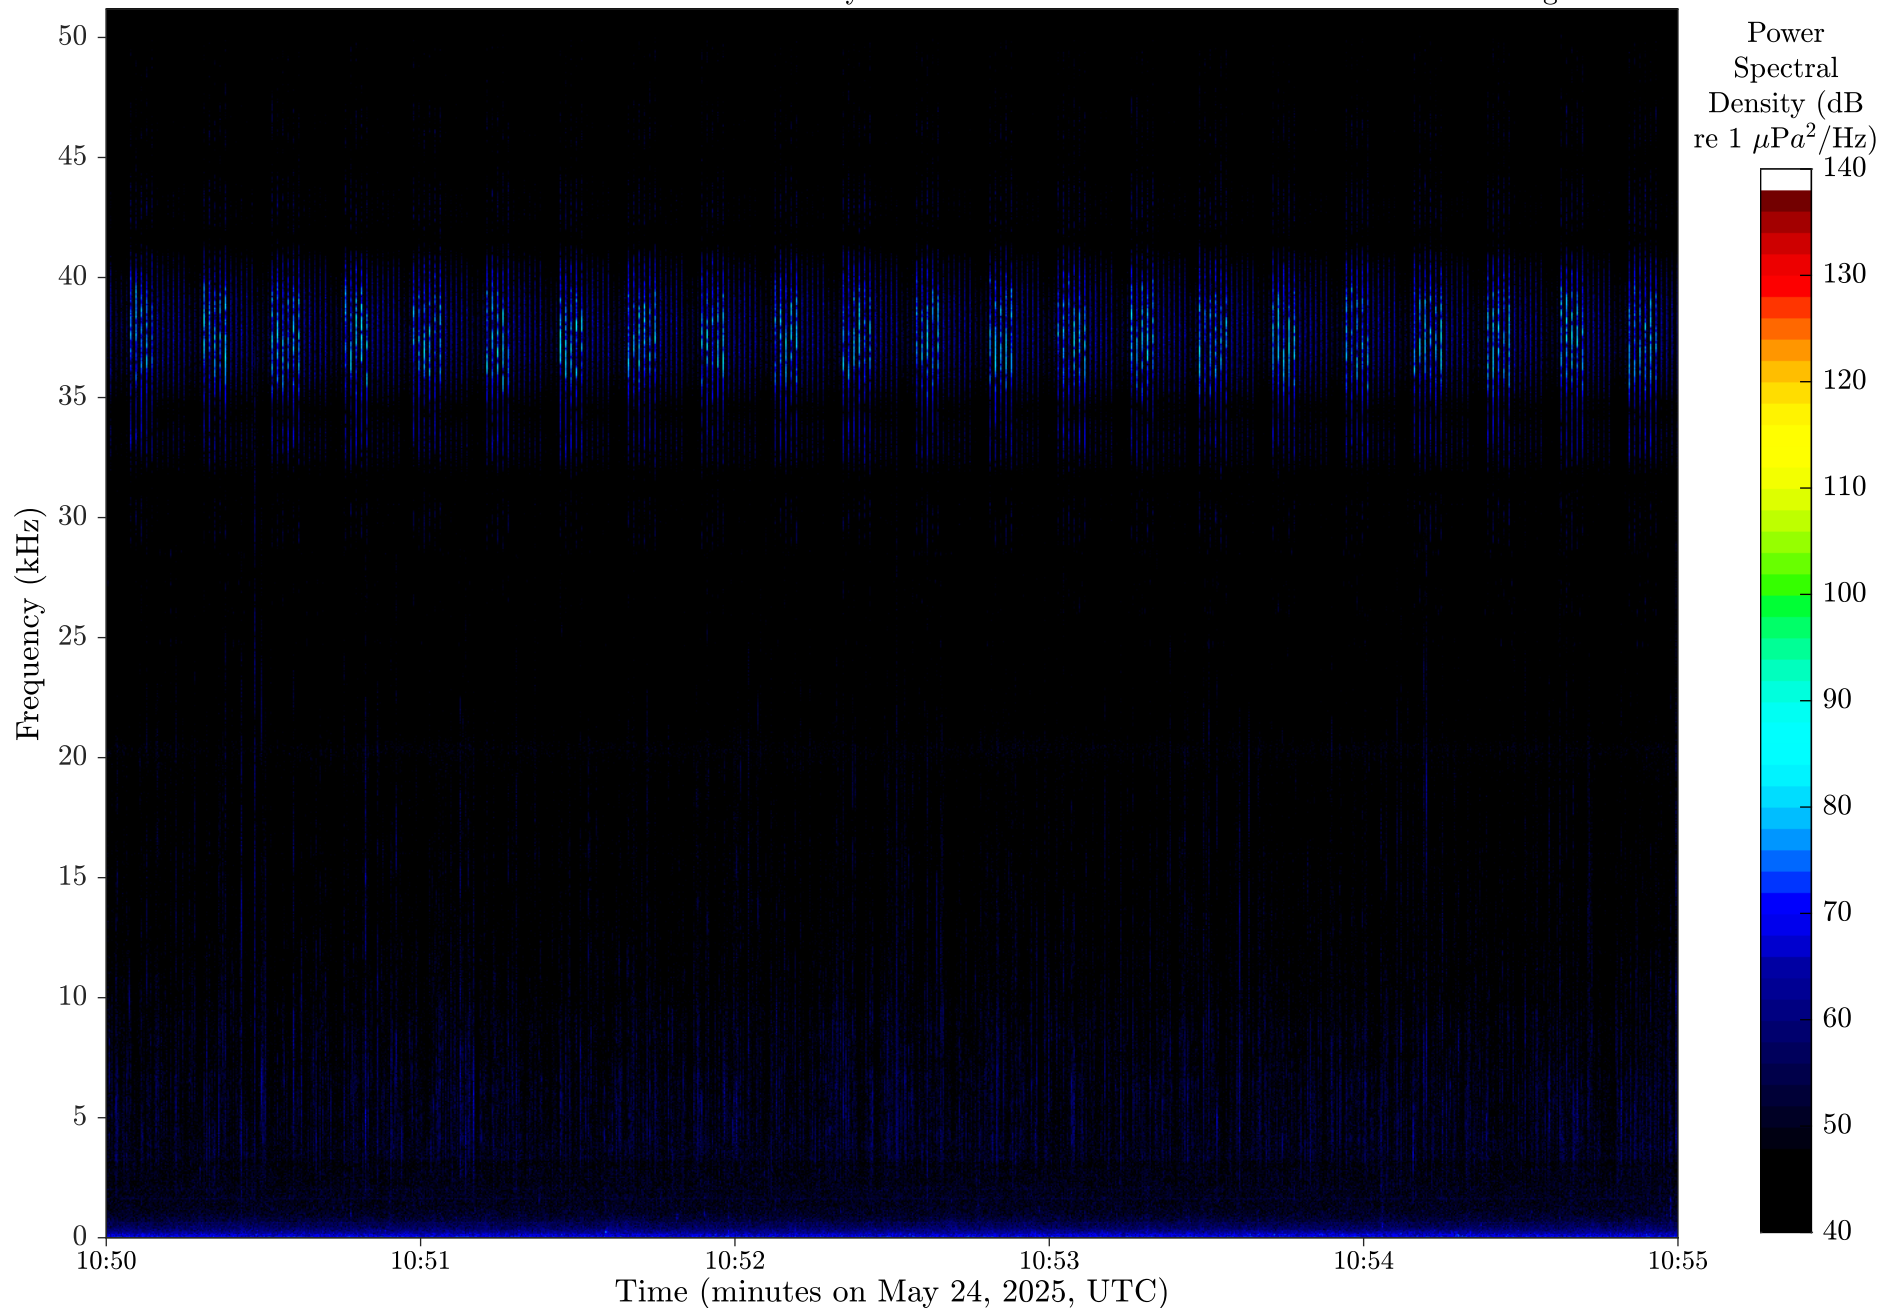


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:33:10 UTC

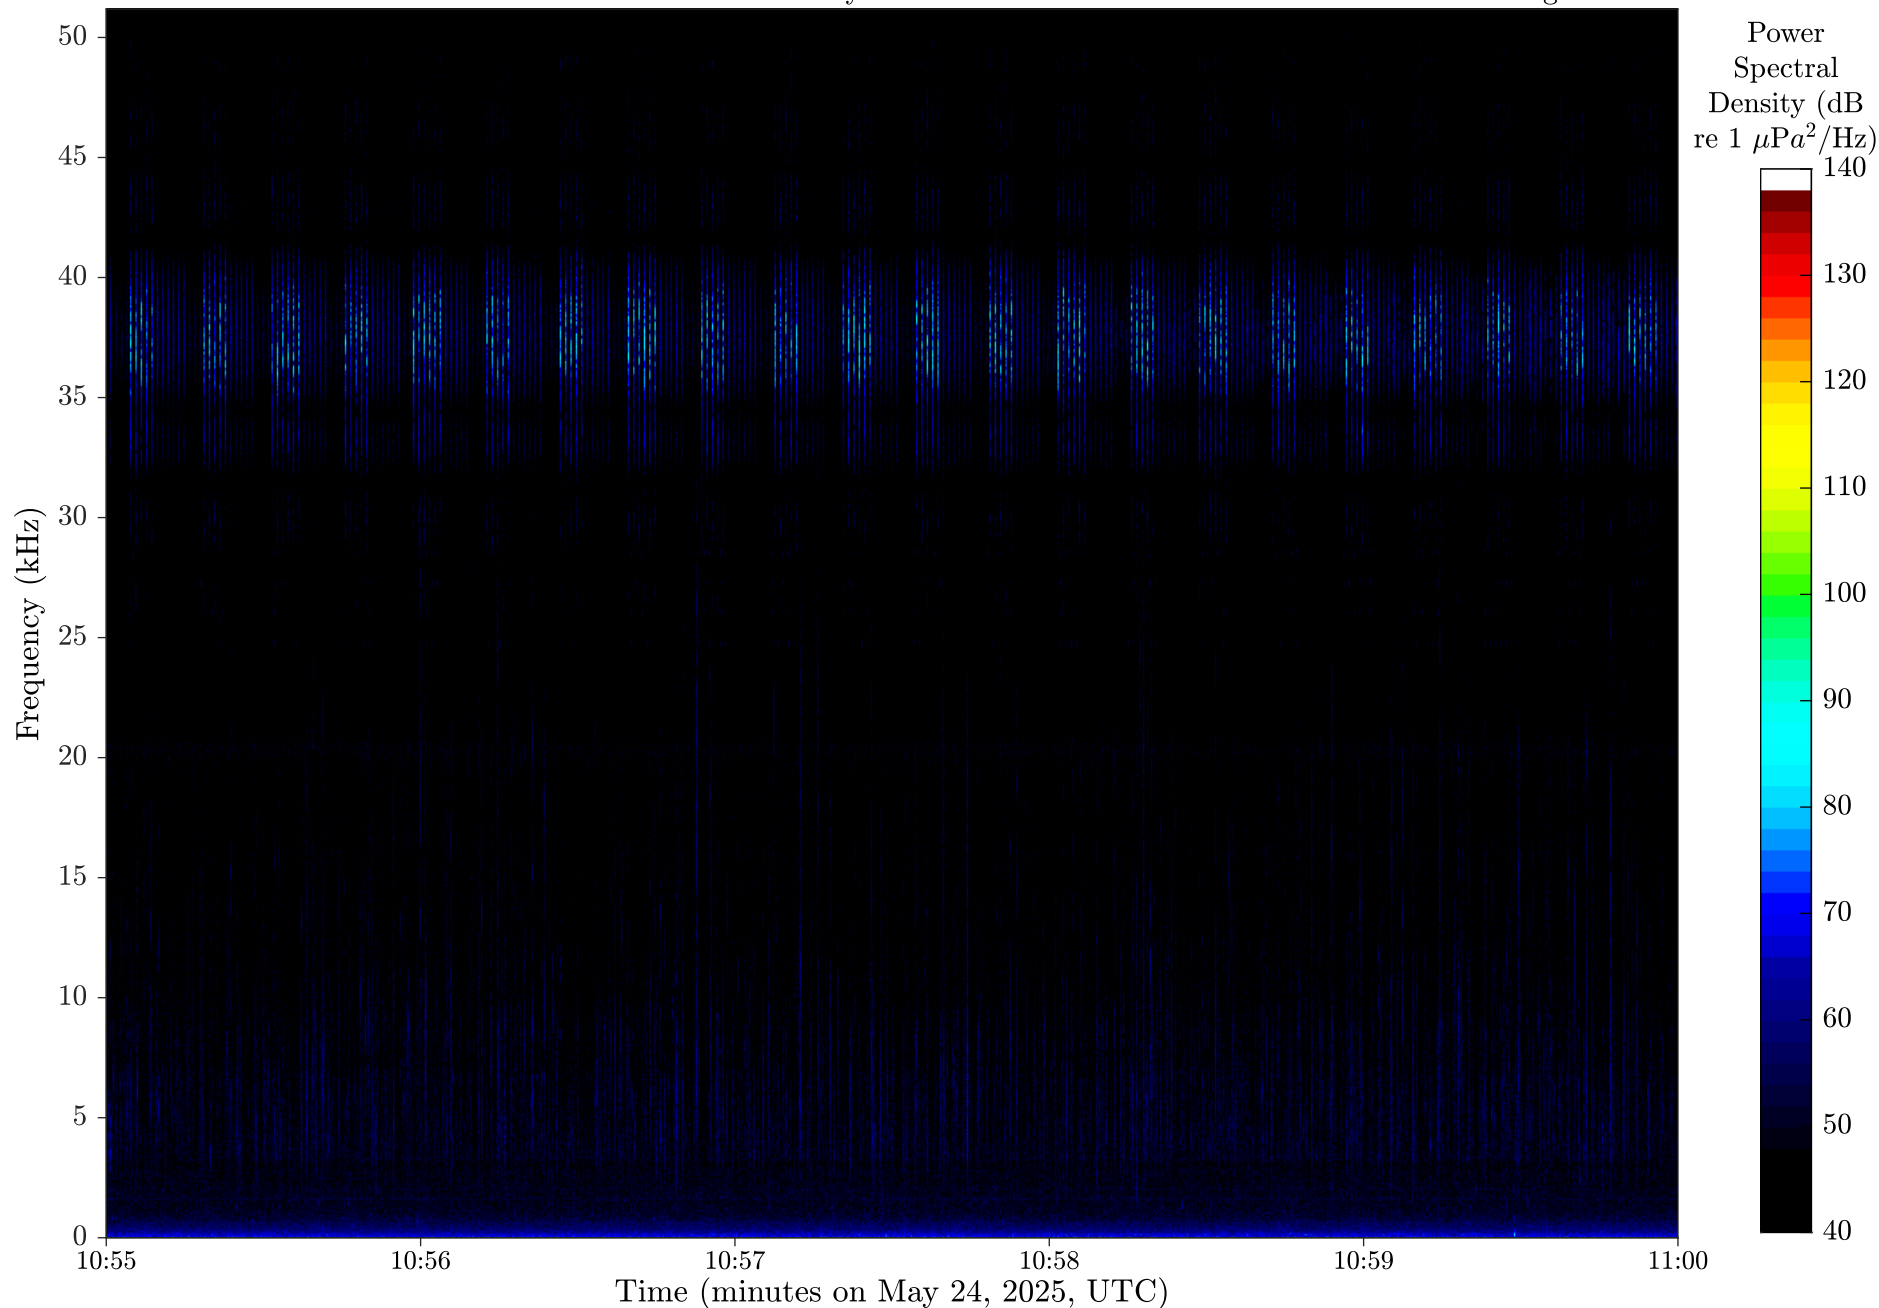

Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:33:21 UTC

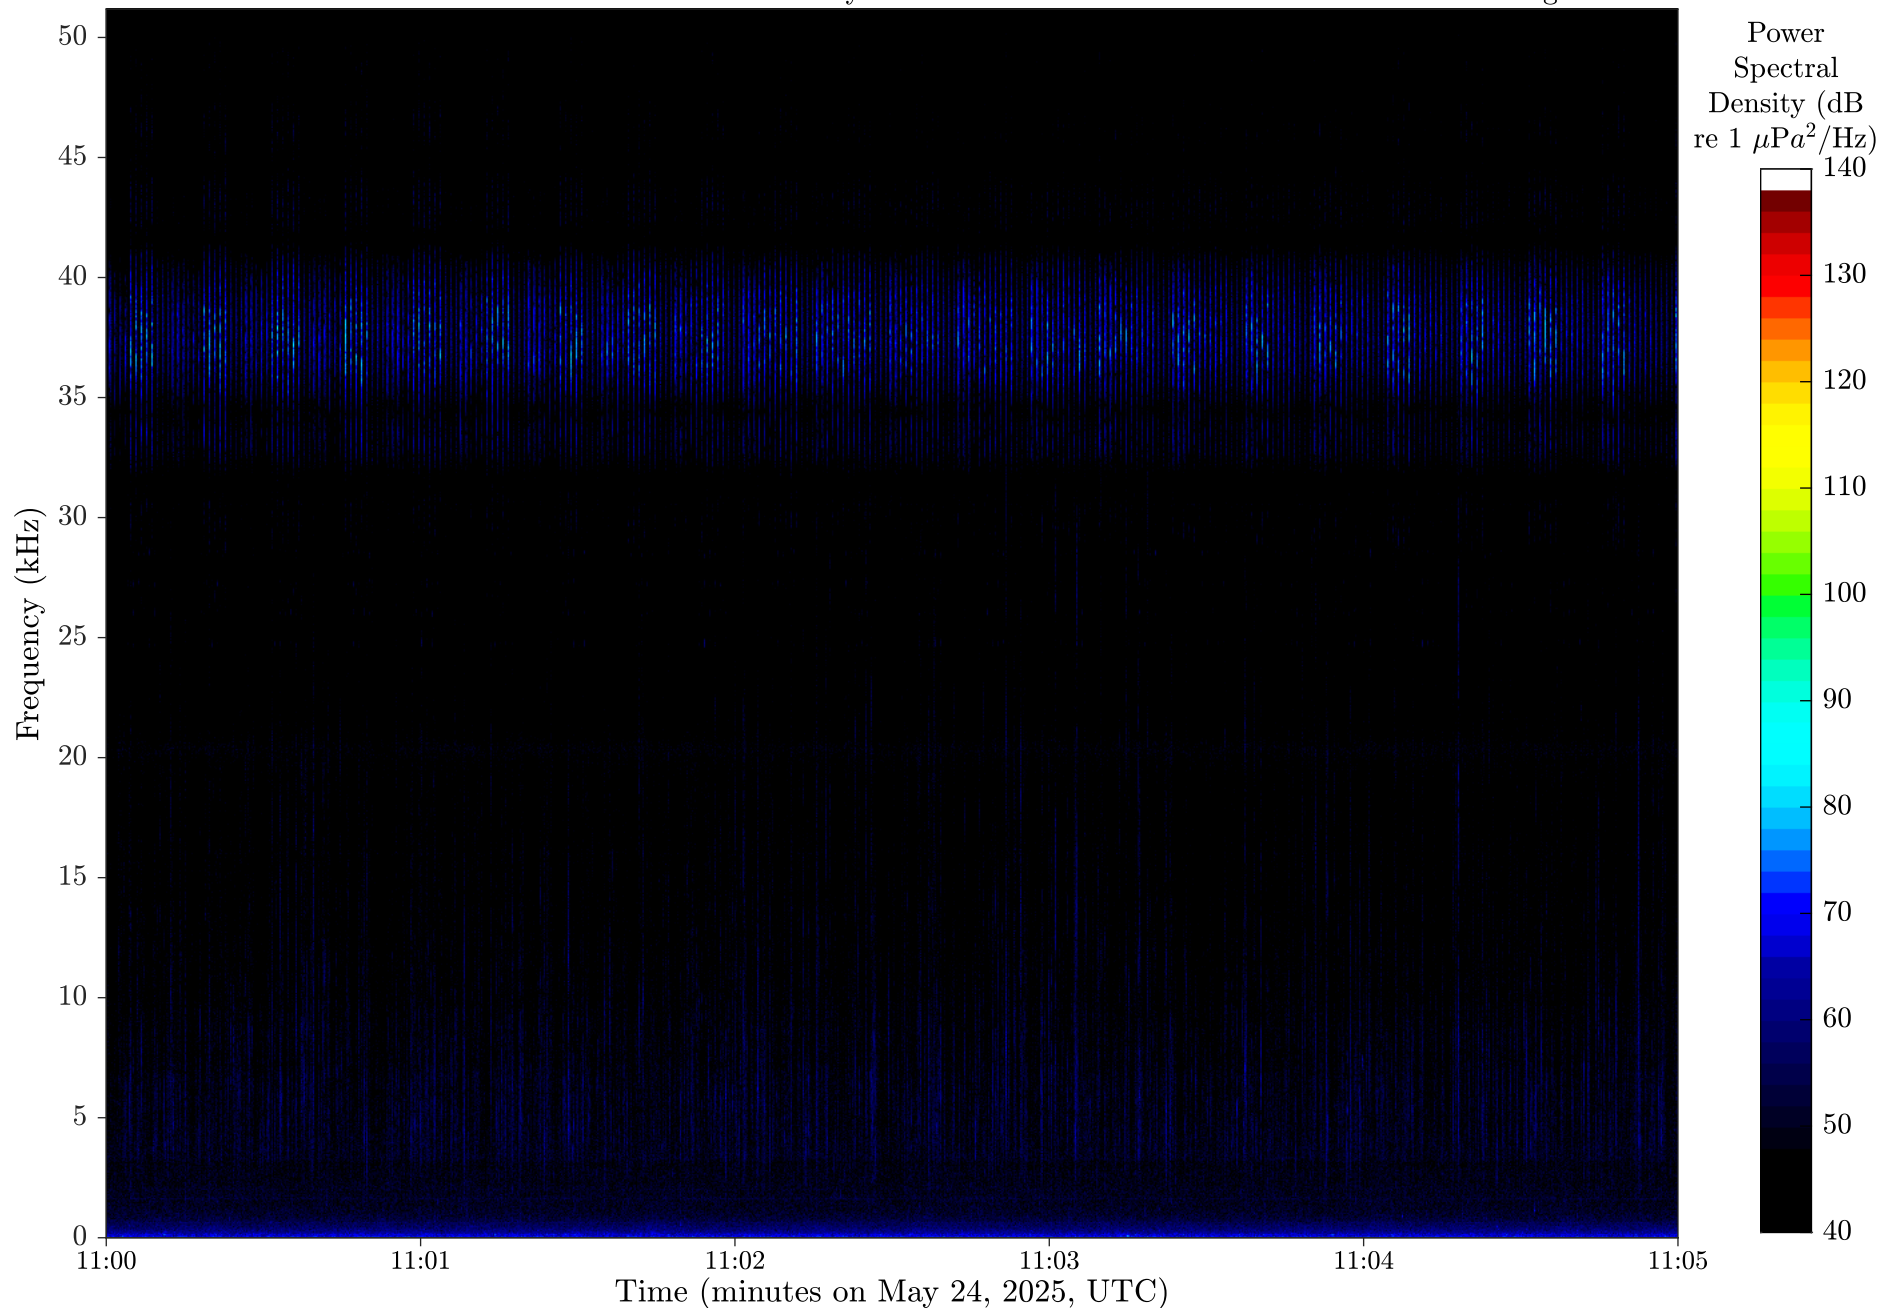

Ocean Sonics icListen HF Hydrophone 1266 (23235)
Folger Passage • Folger Deep • 48.8139° N • 125.2746° W • 95 m
Start time: 24-May-2025 11:05:00.000 UTC • Data Diversion Mode: Original Data




Comments: 23.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

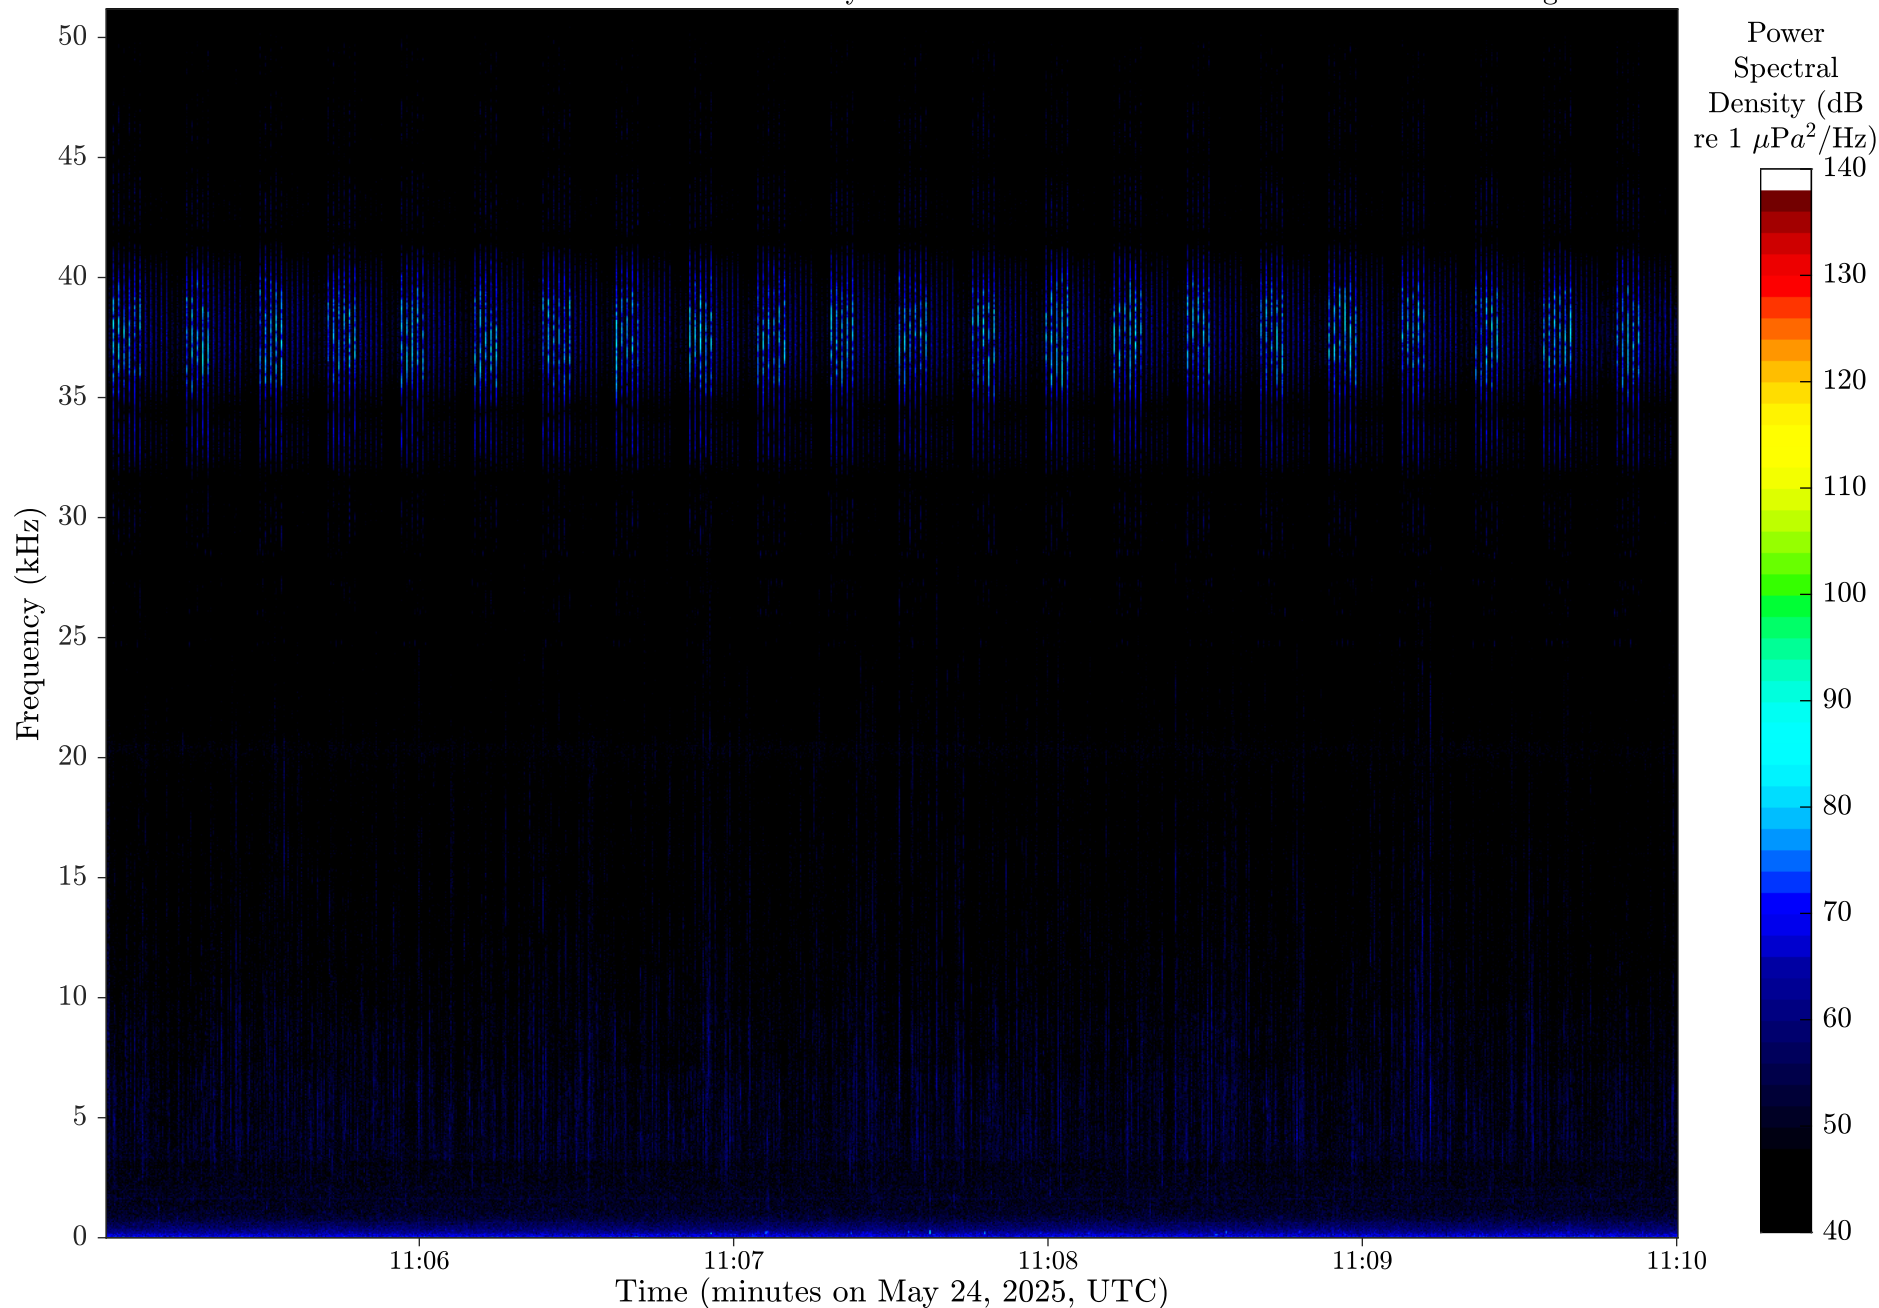


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:33:39 UTC

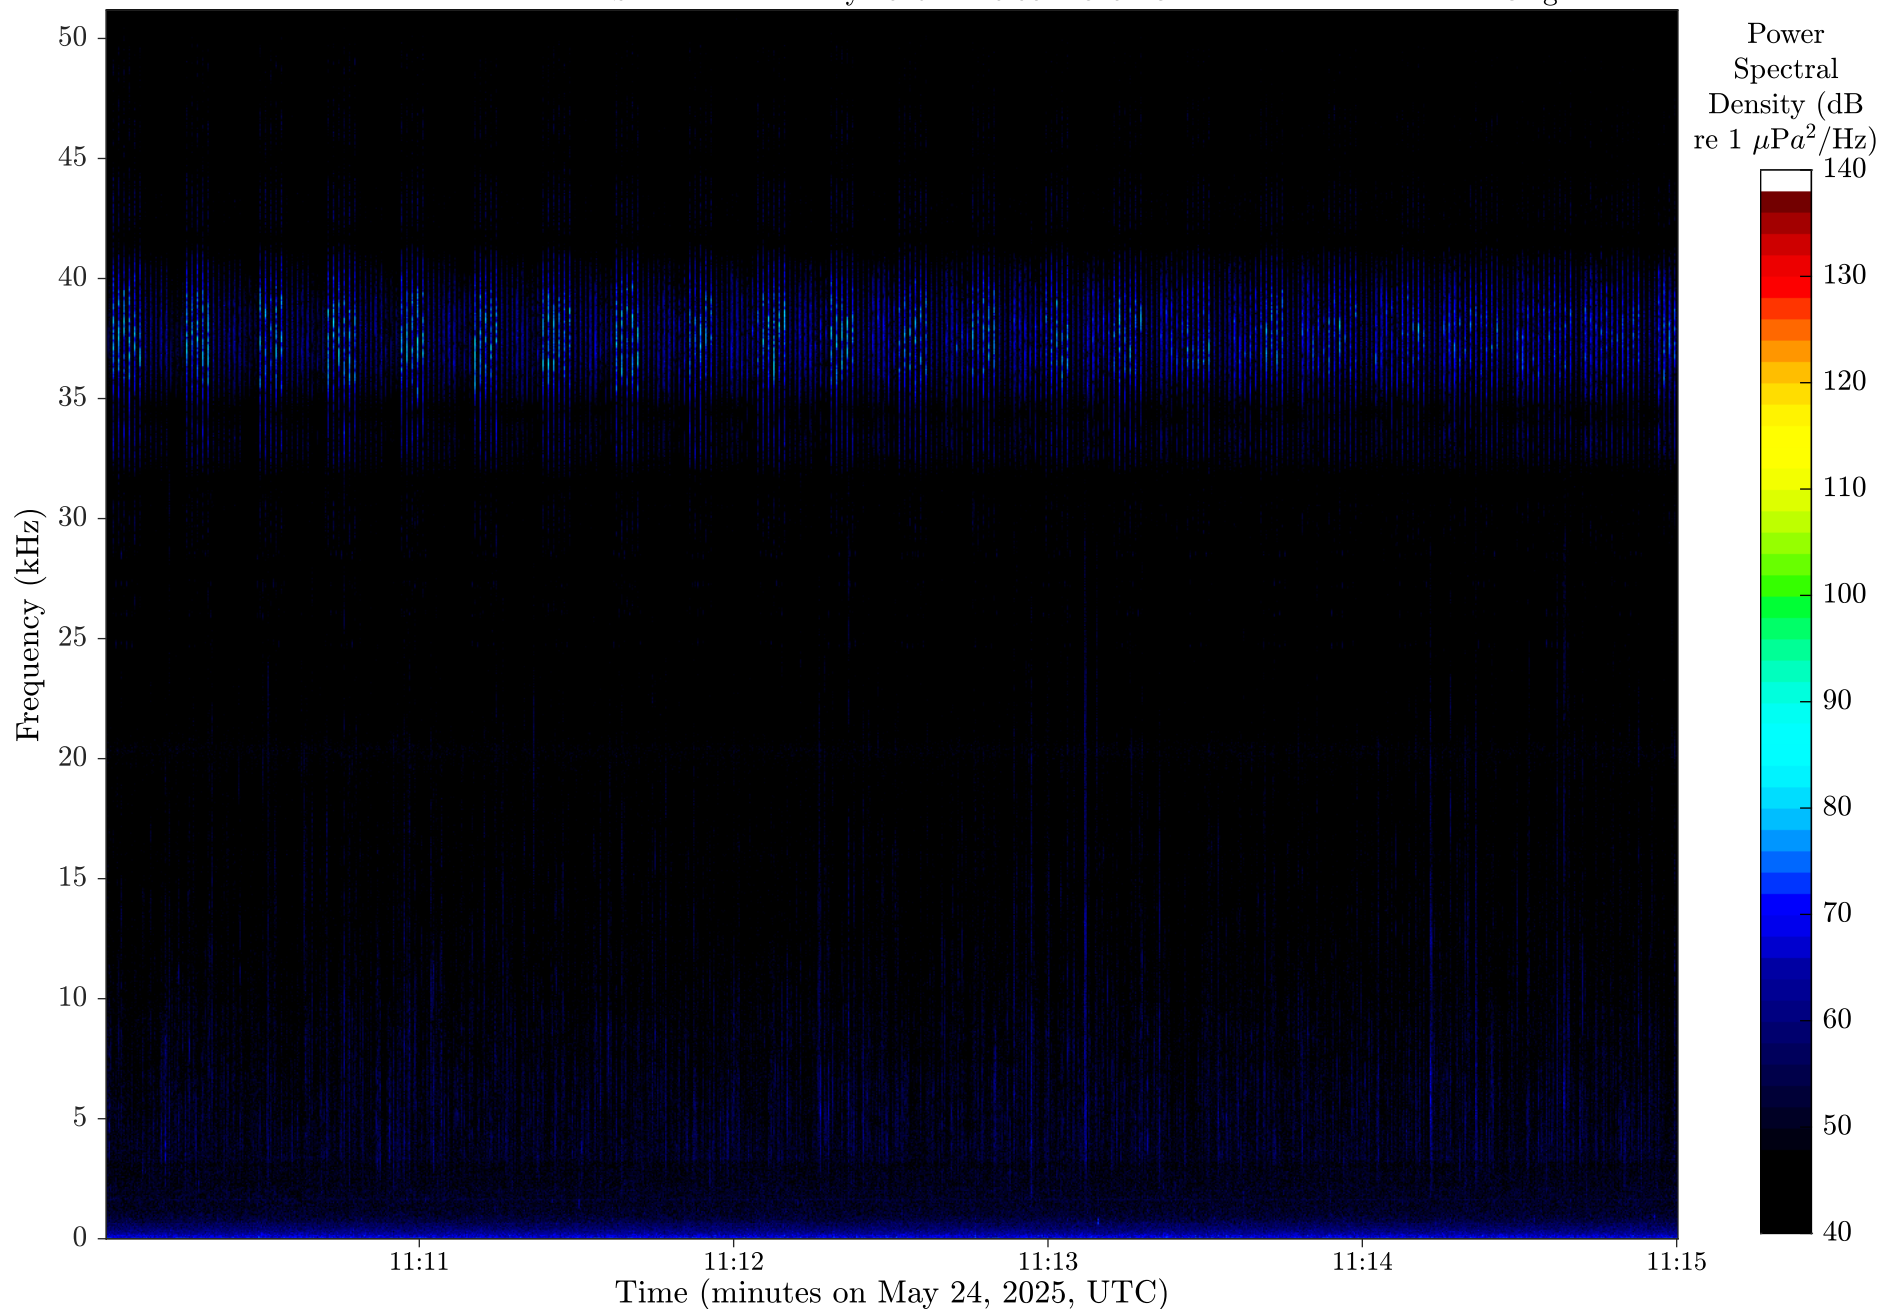


Comments: 32.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:33:47 UTC

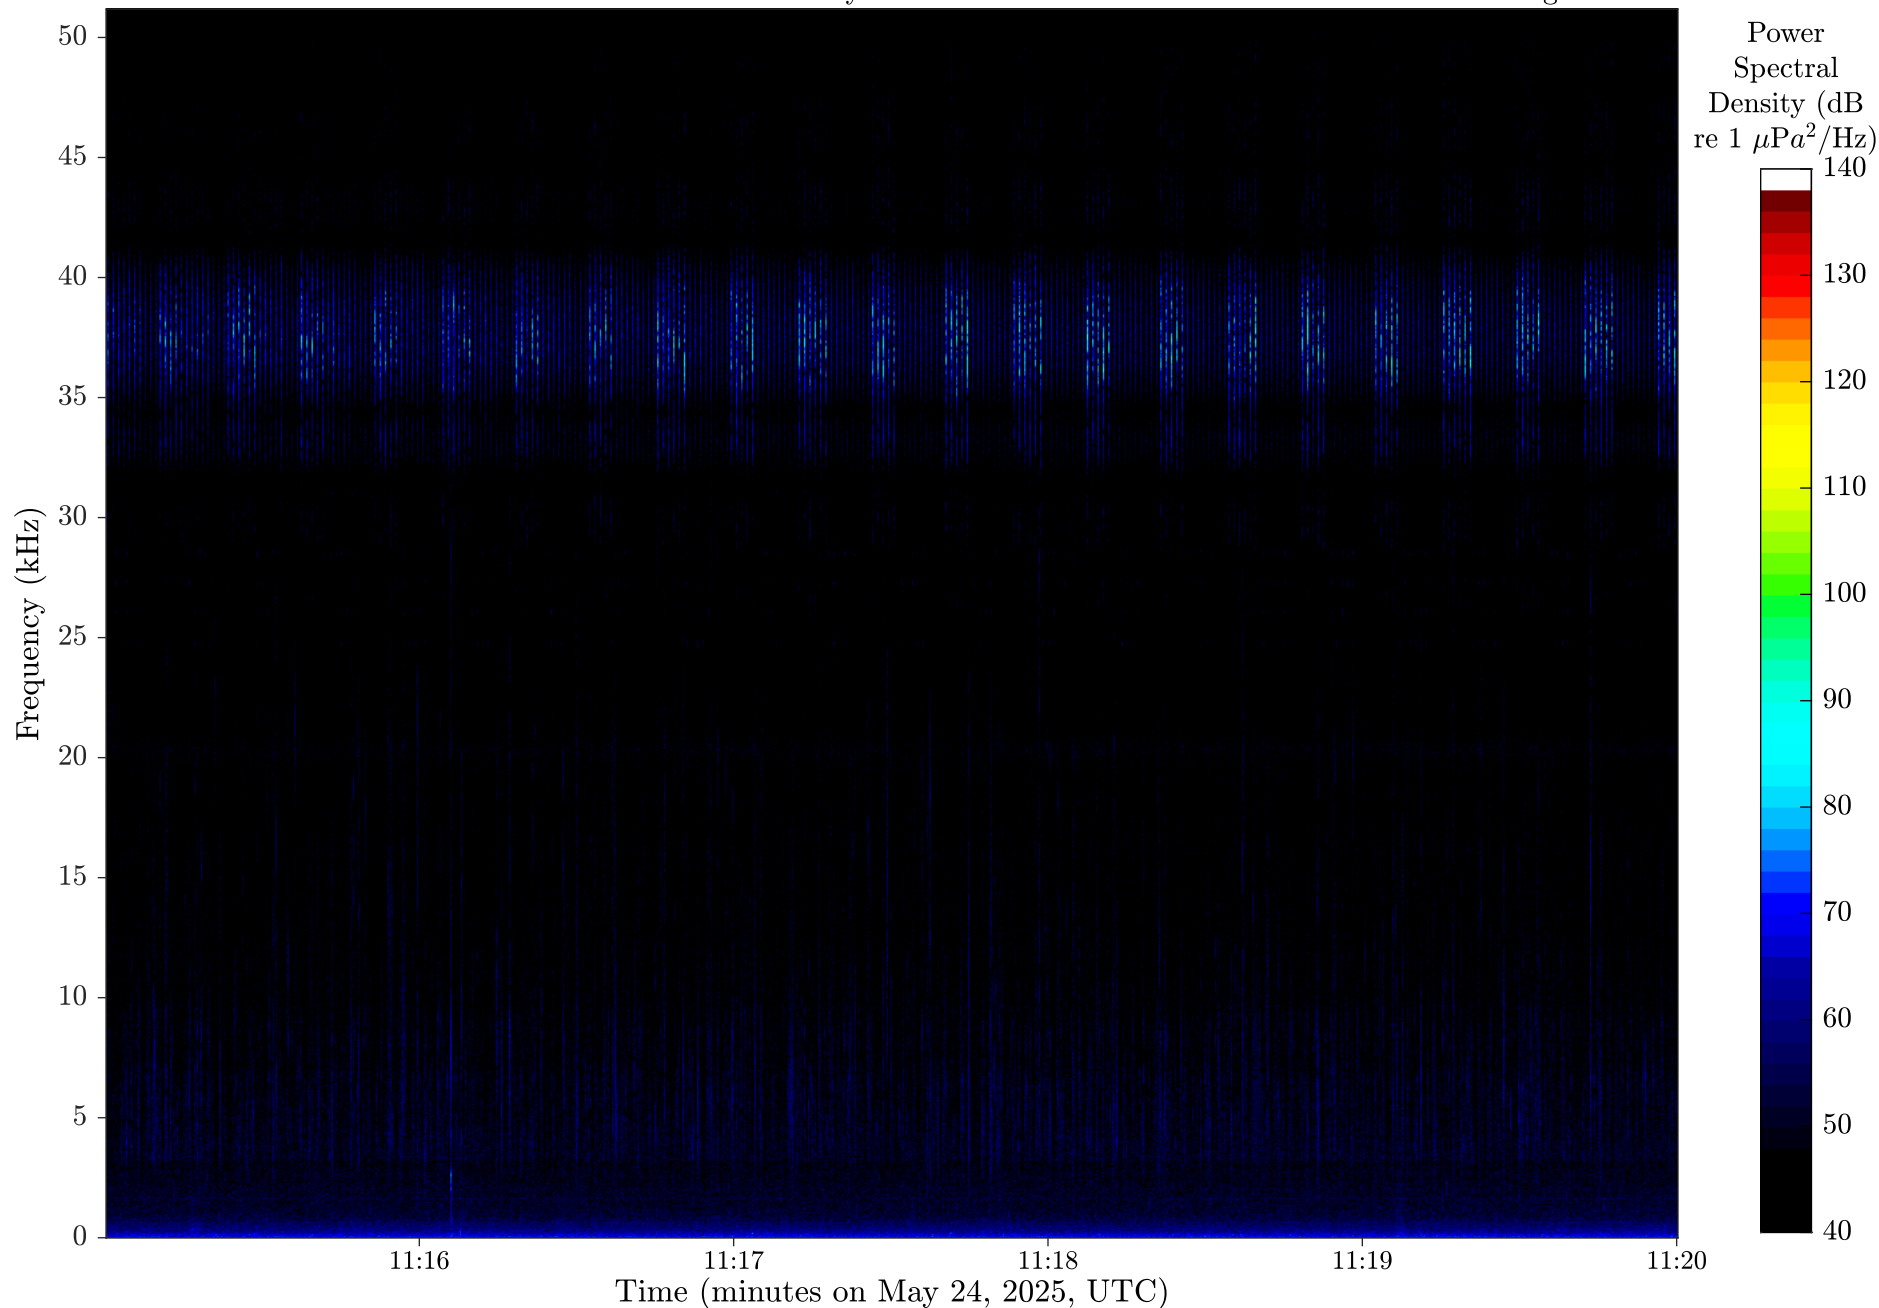


Comments: 31.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:33:55 UTC

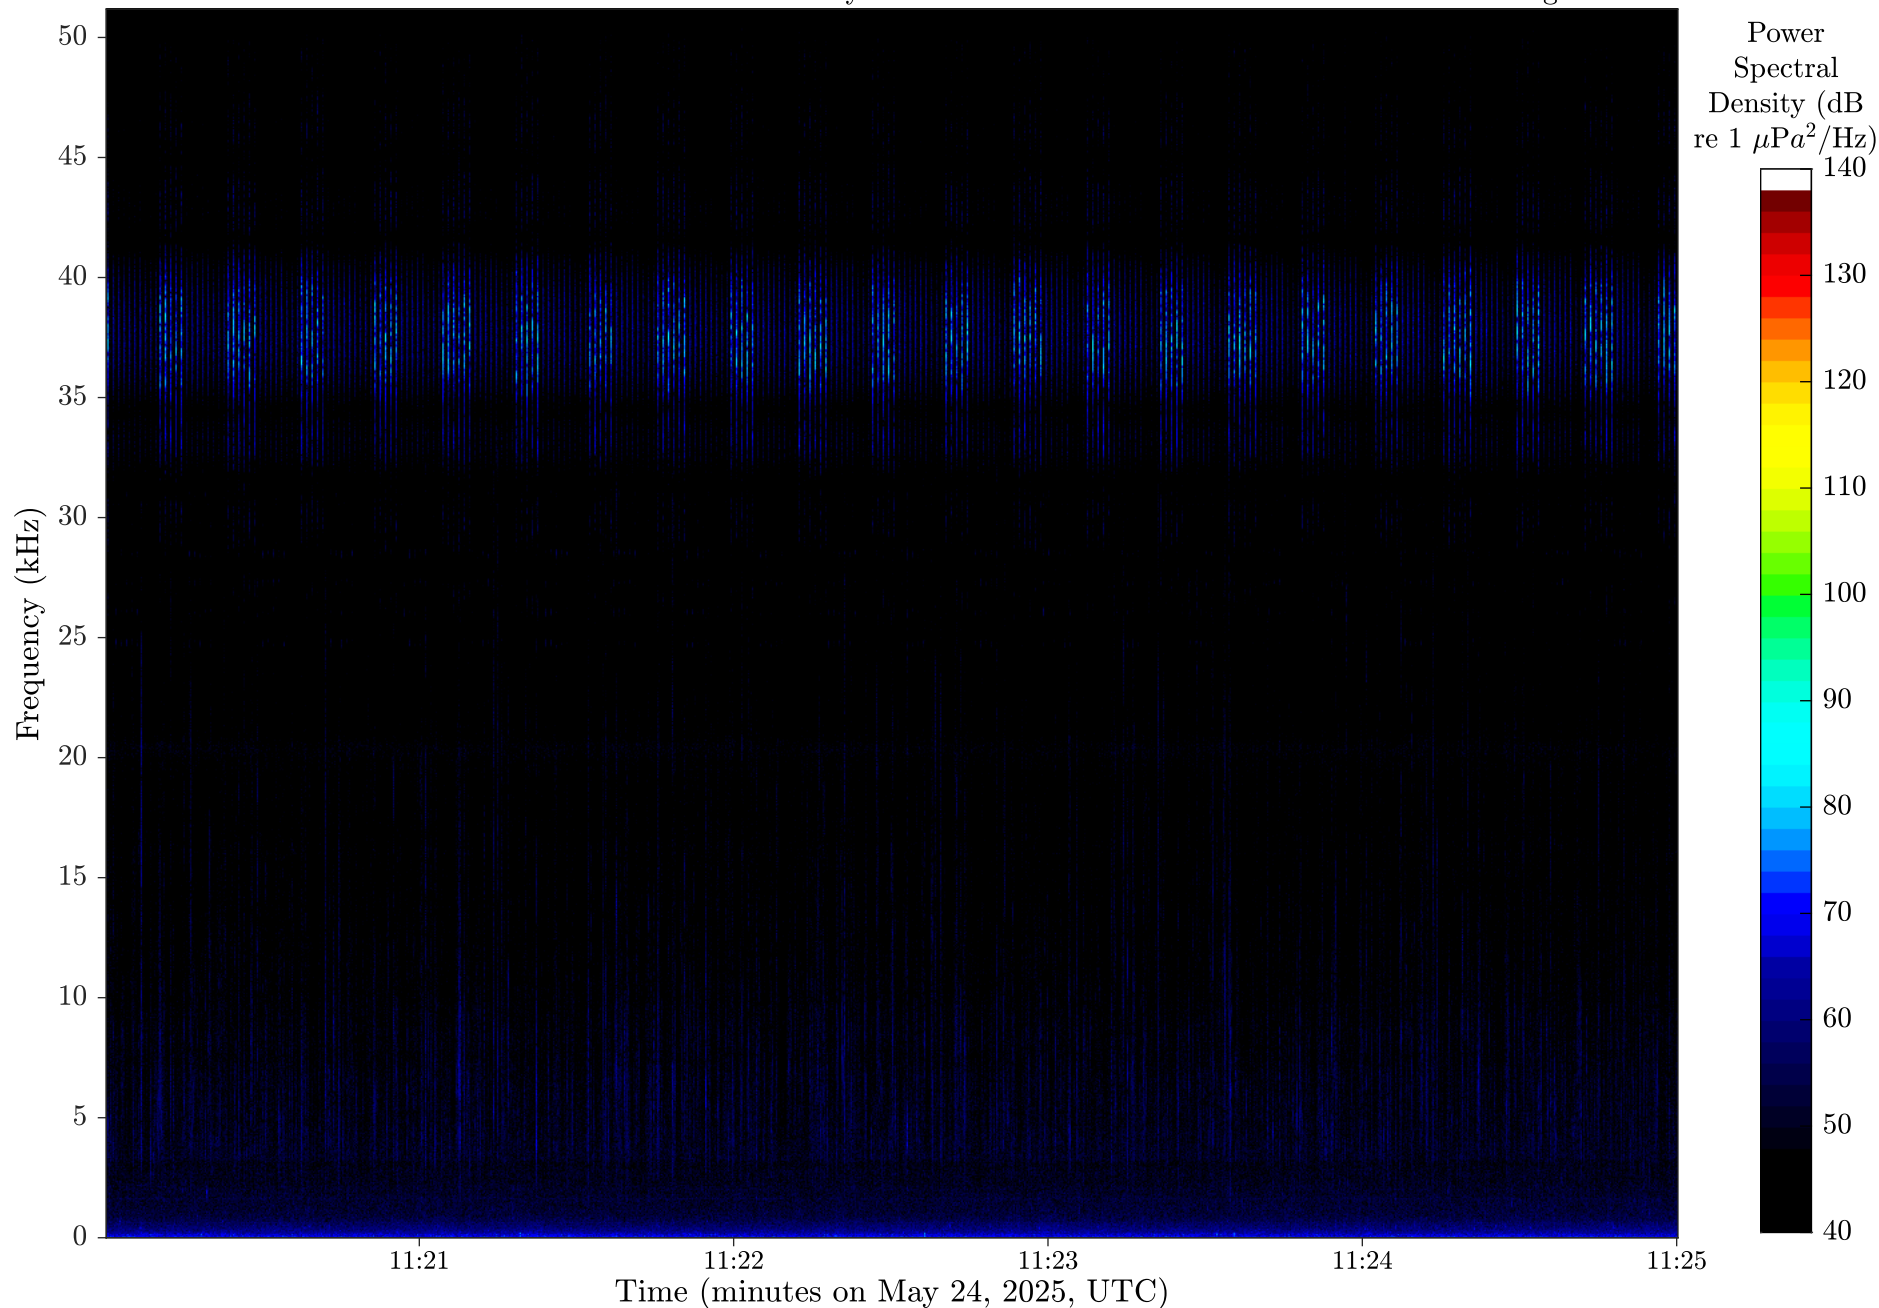


Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:03 UTC

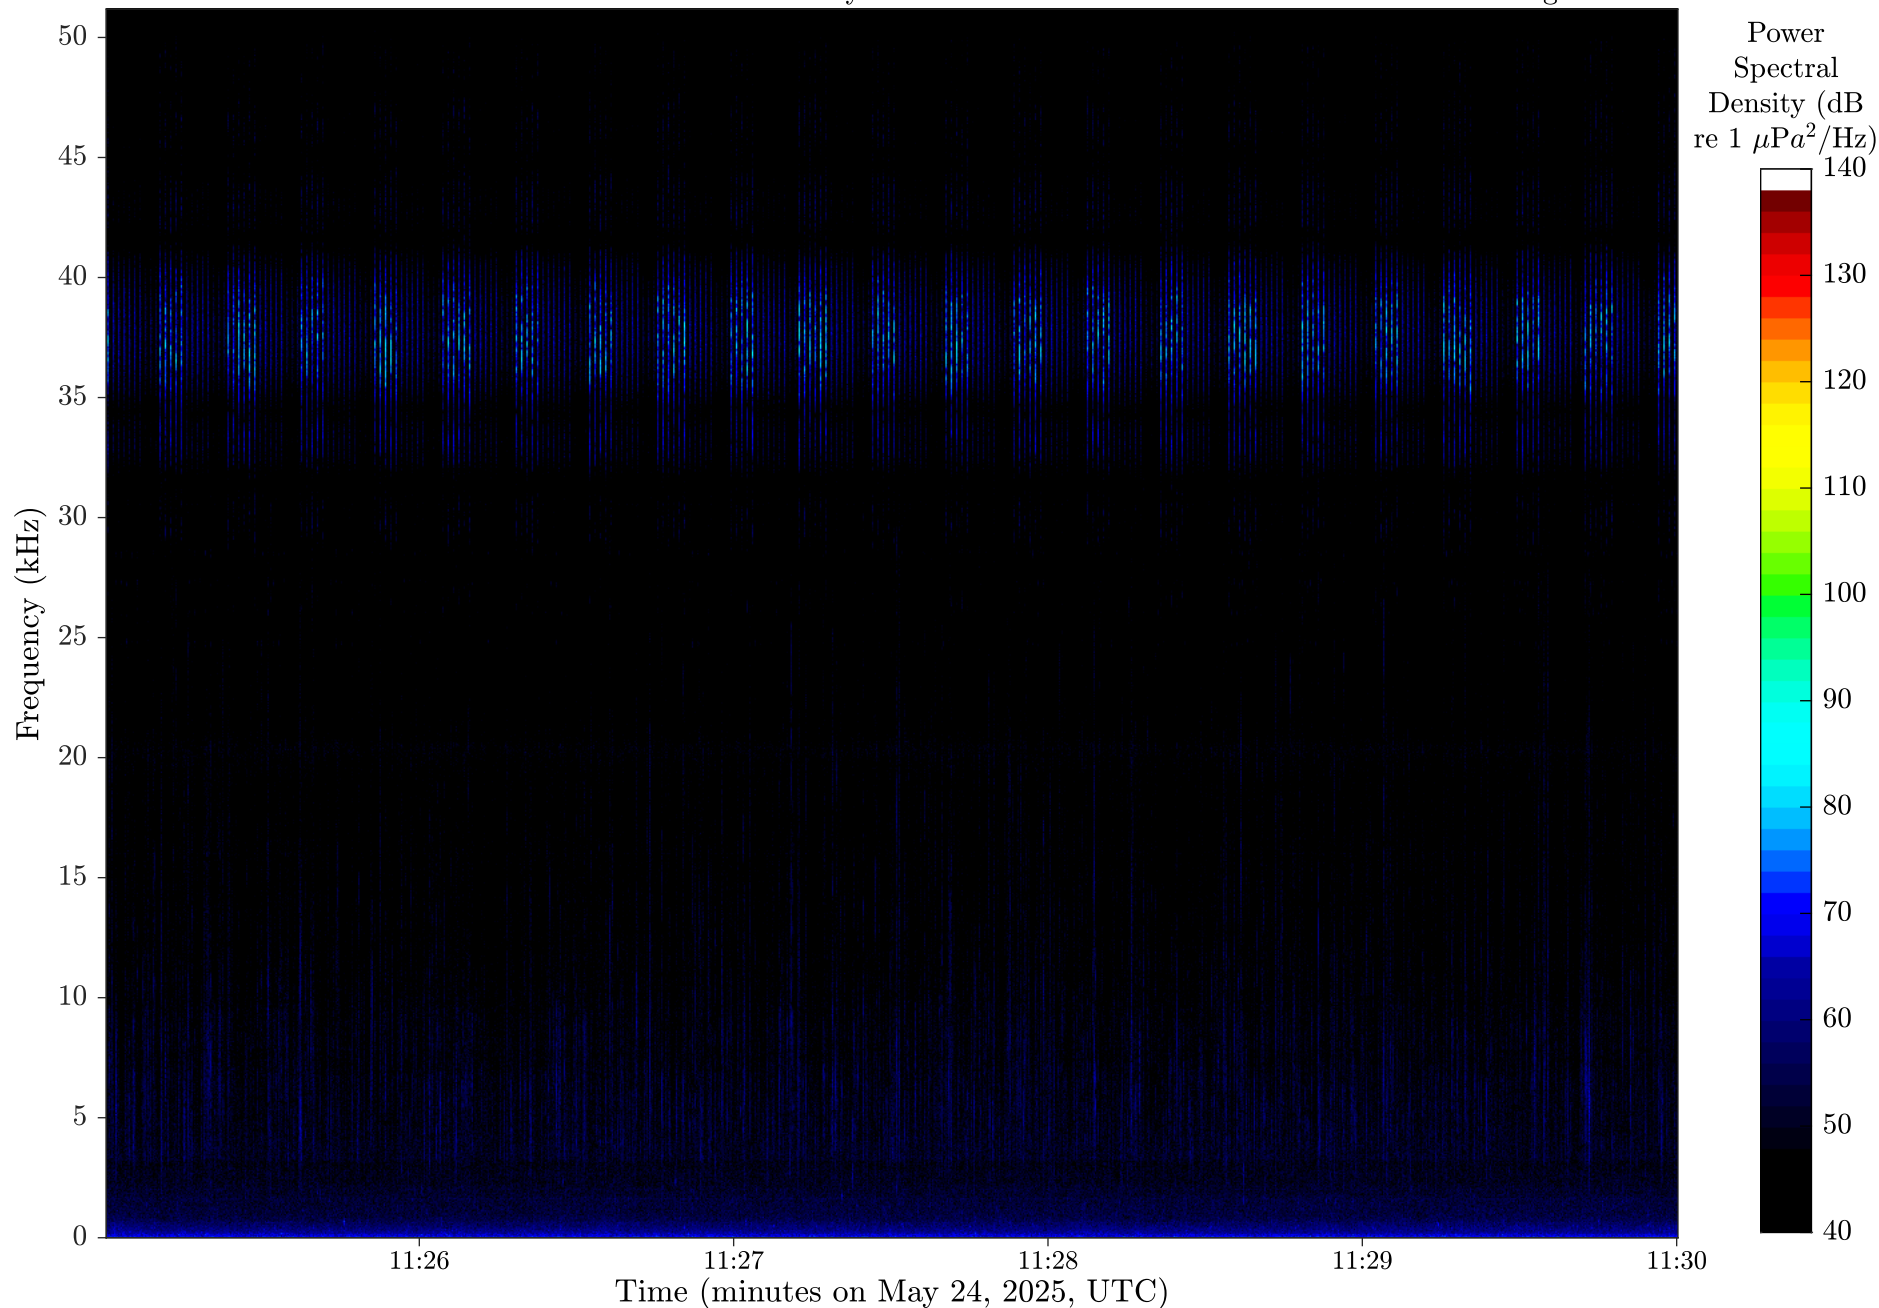


Comments: 32.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:11 UTC

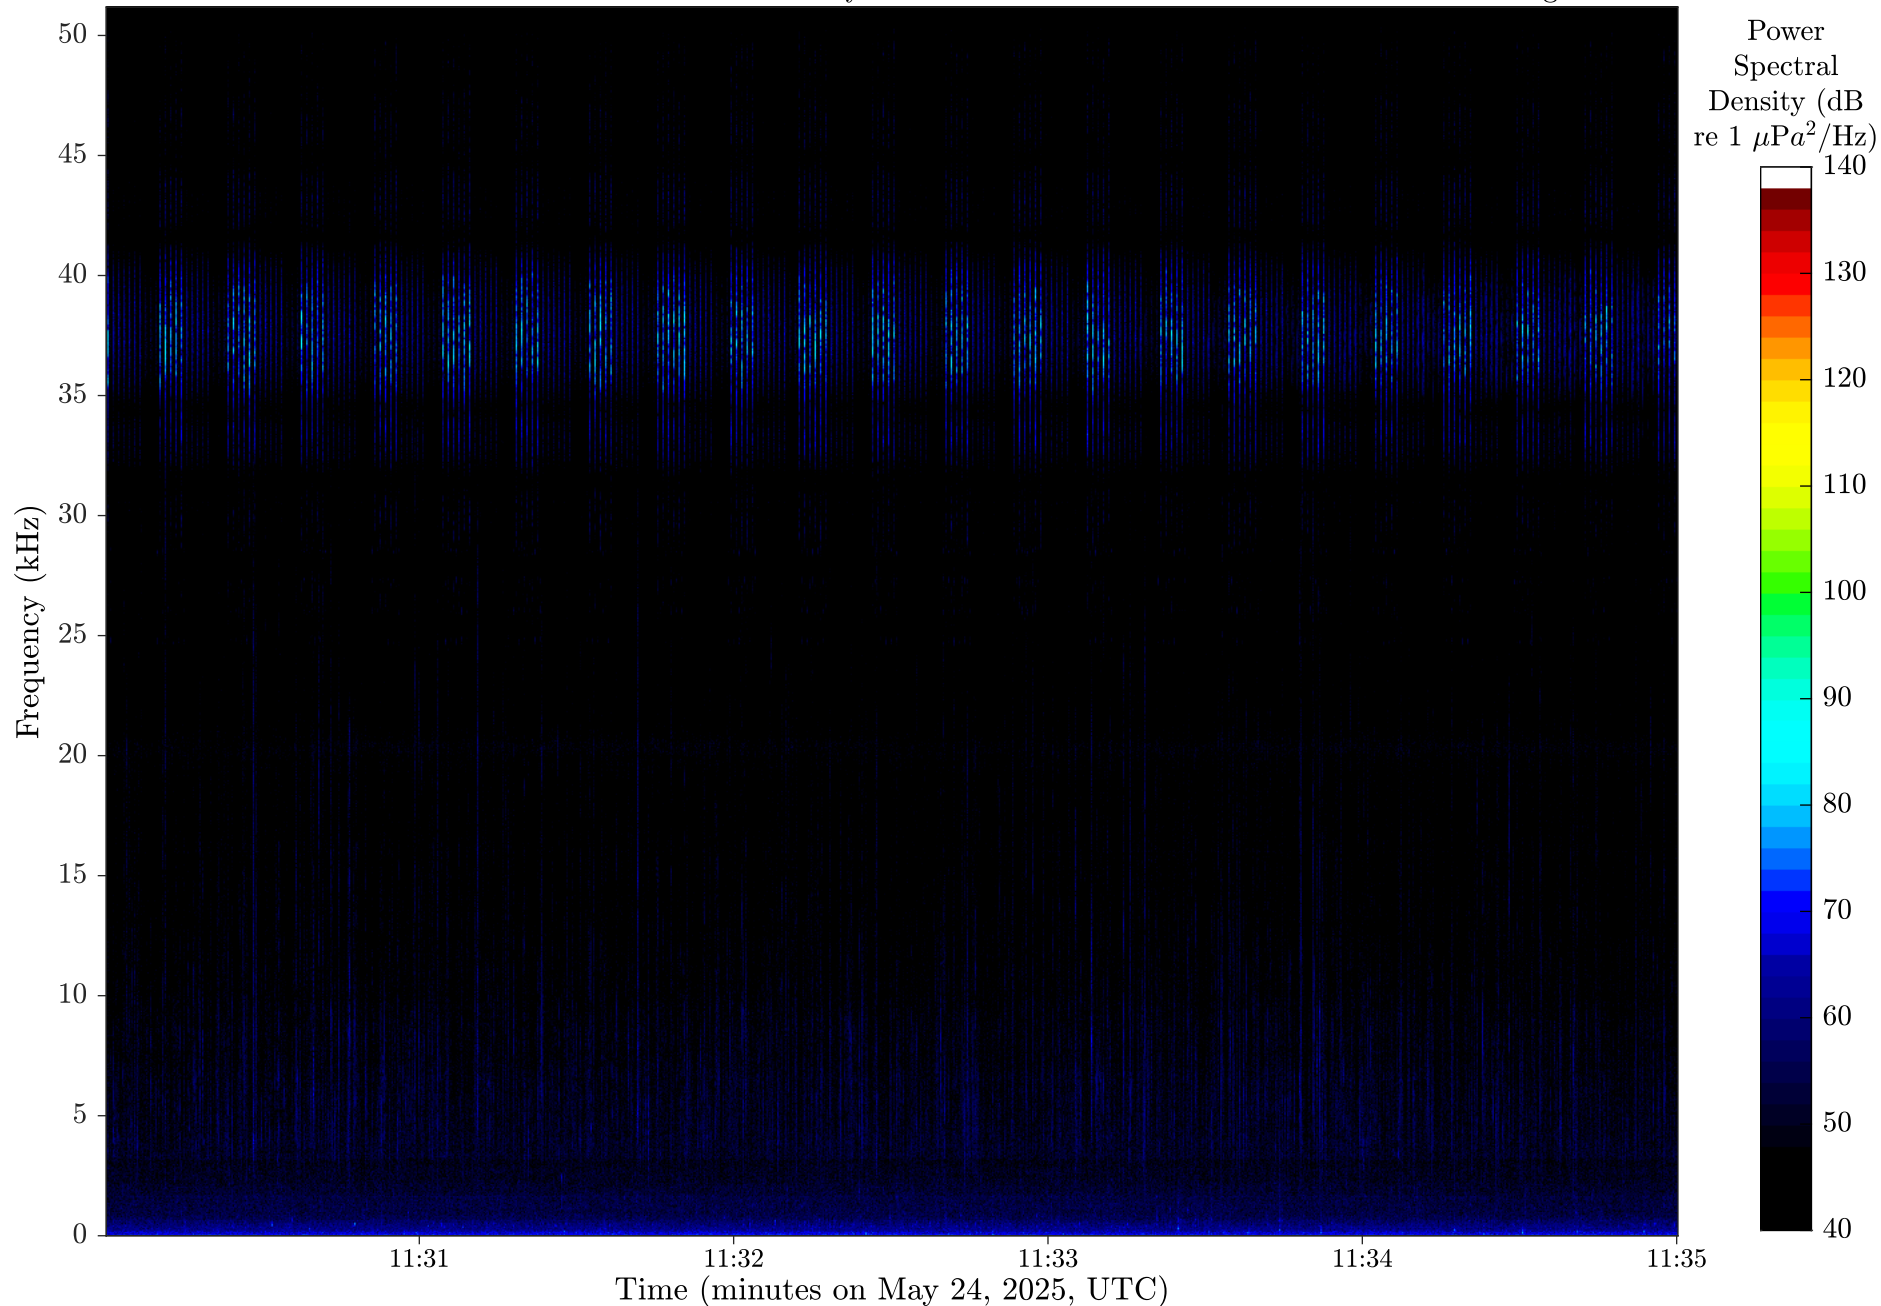


Comments: 32.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:19 UTC

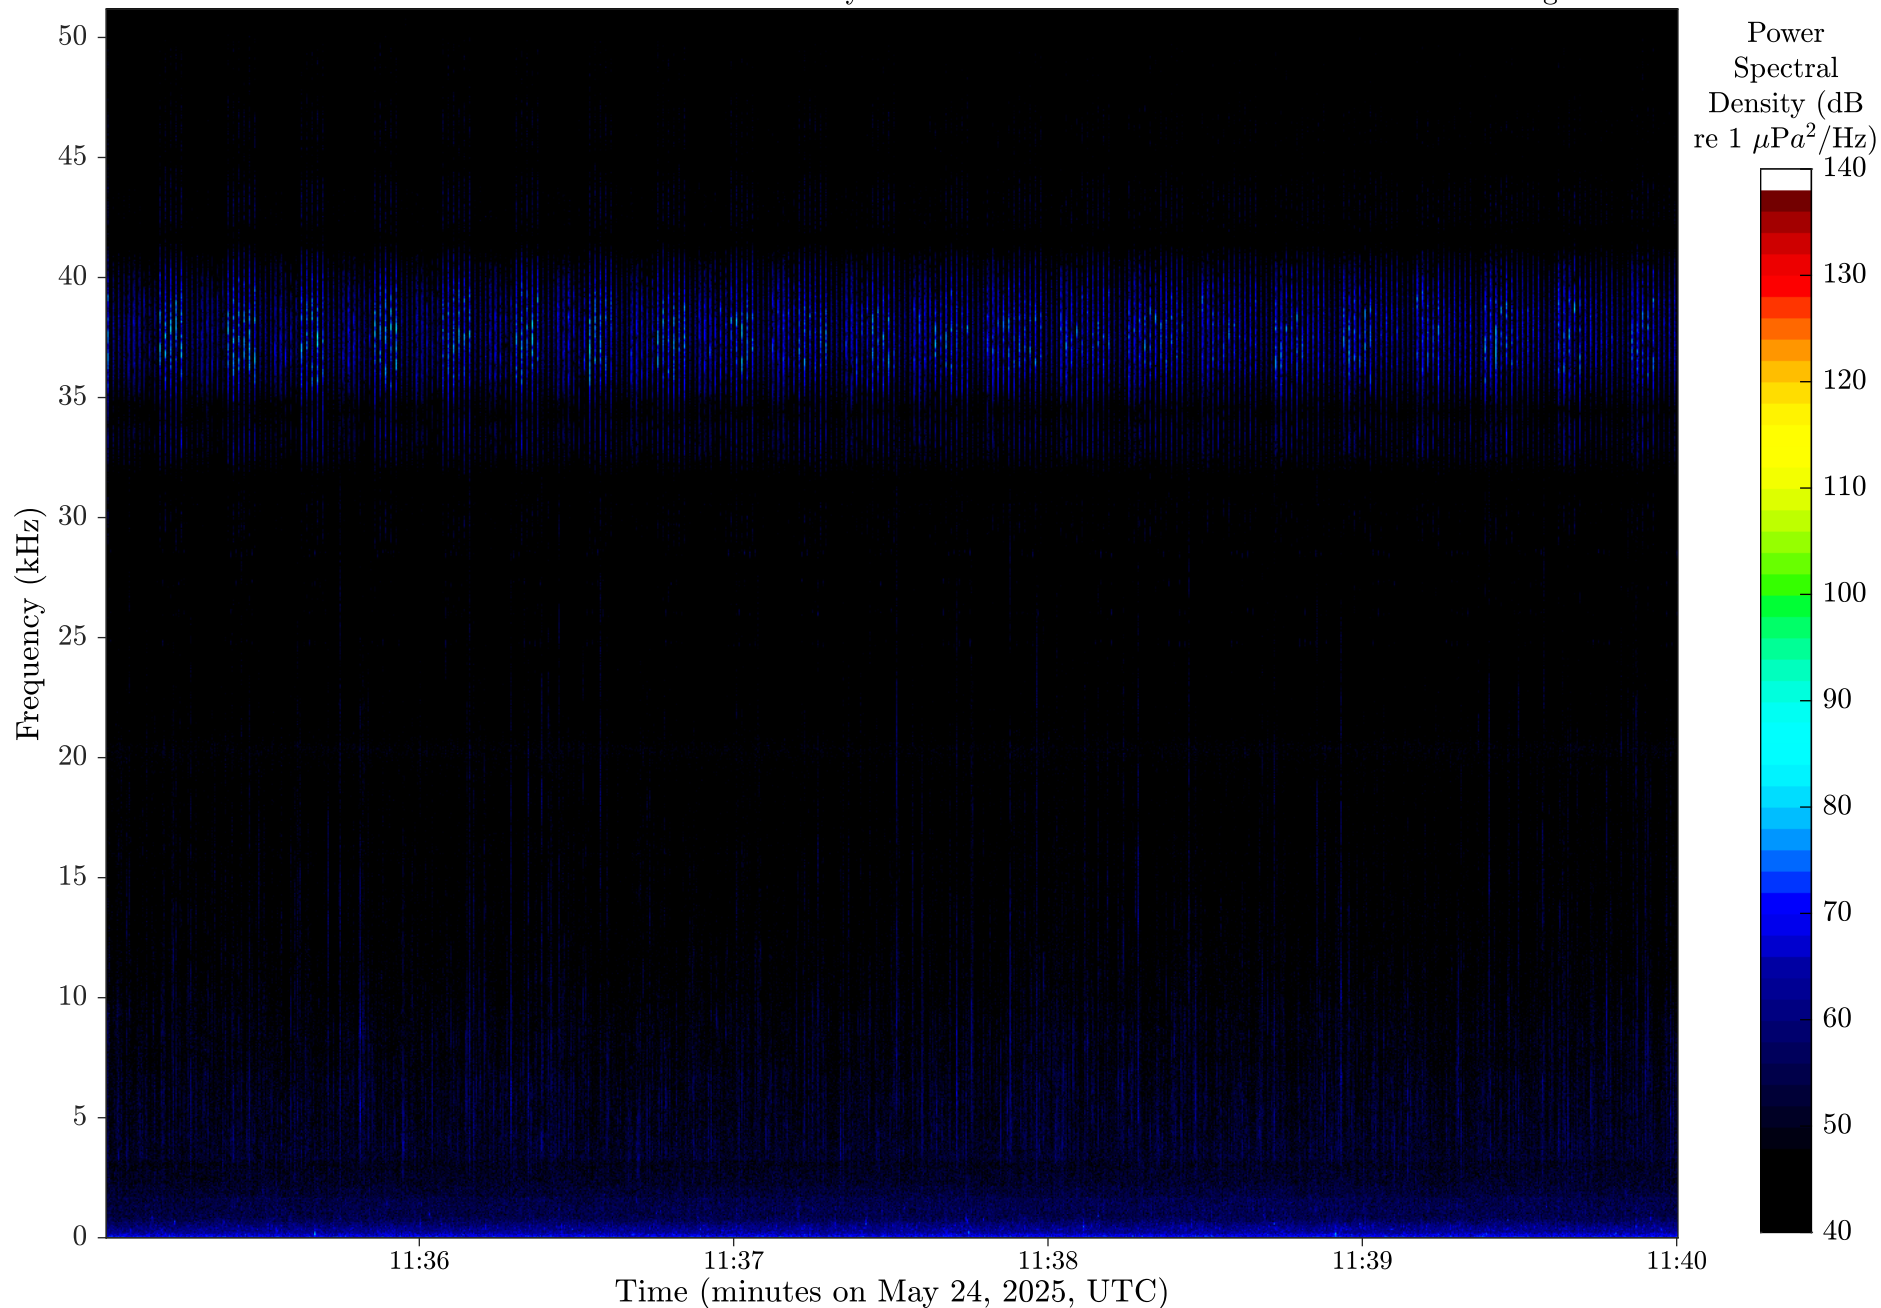


Comments: 30.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:26 UTC

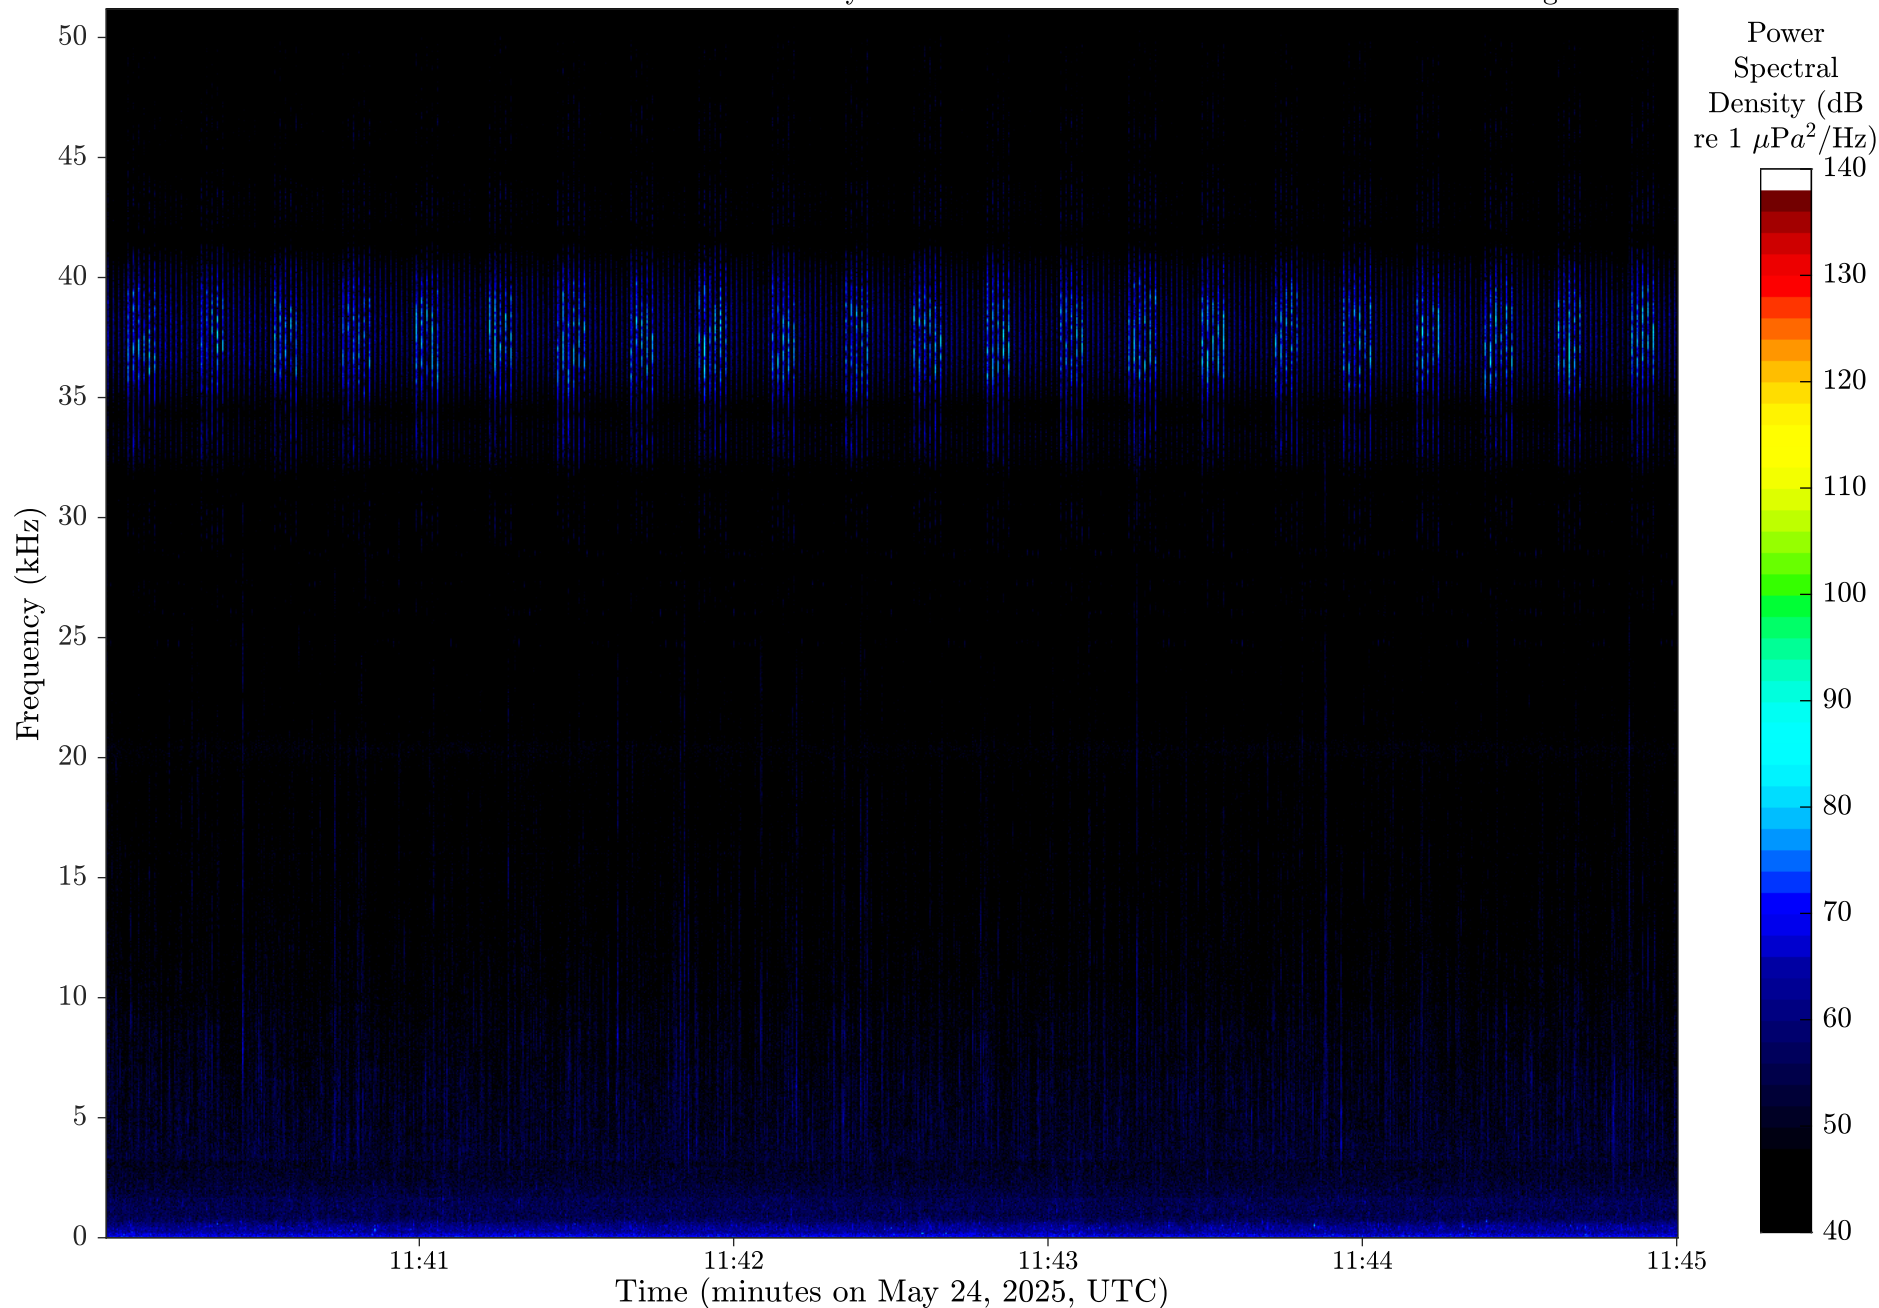


Comments: 30.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:35 UTC

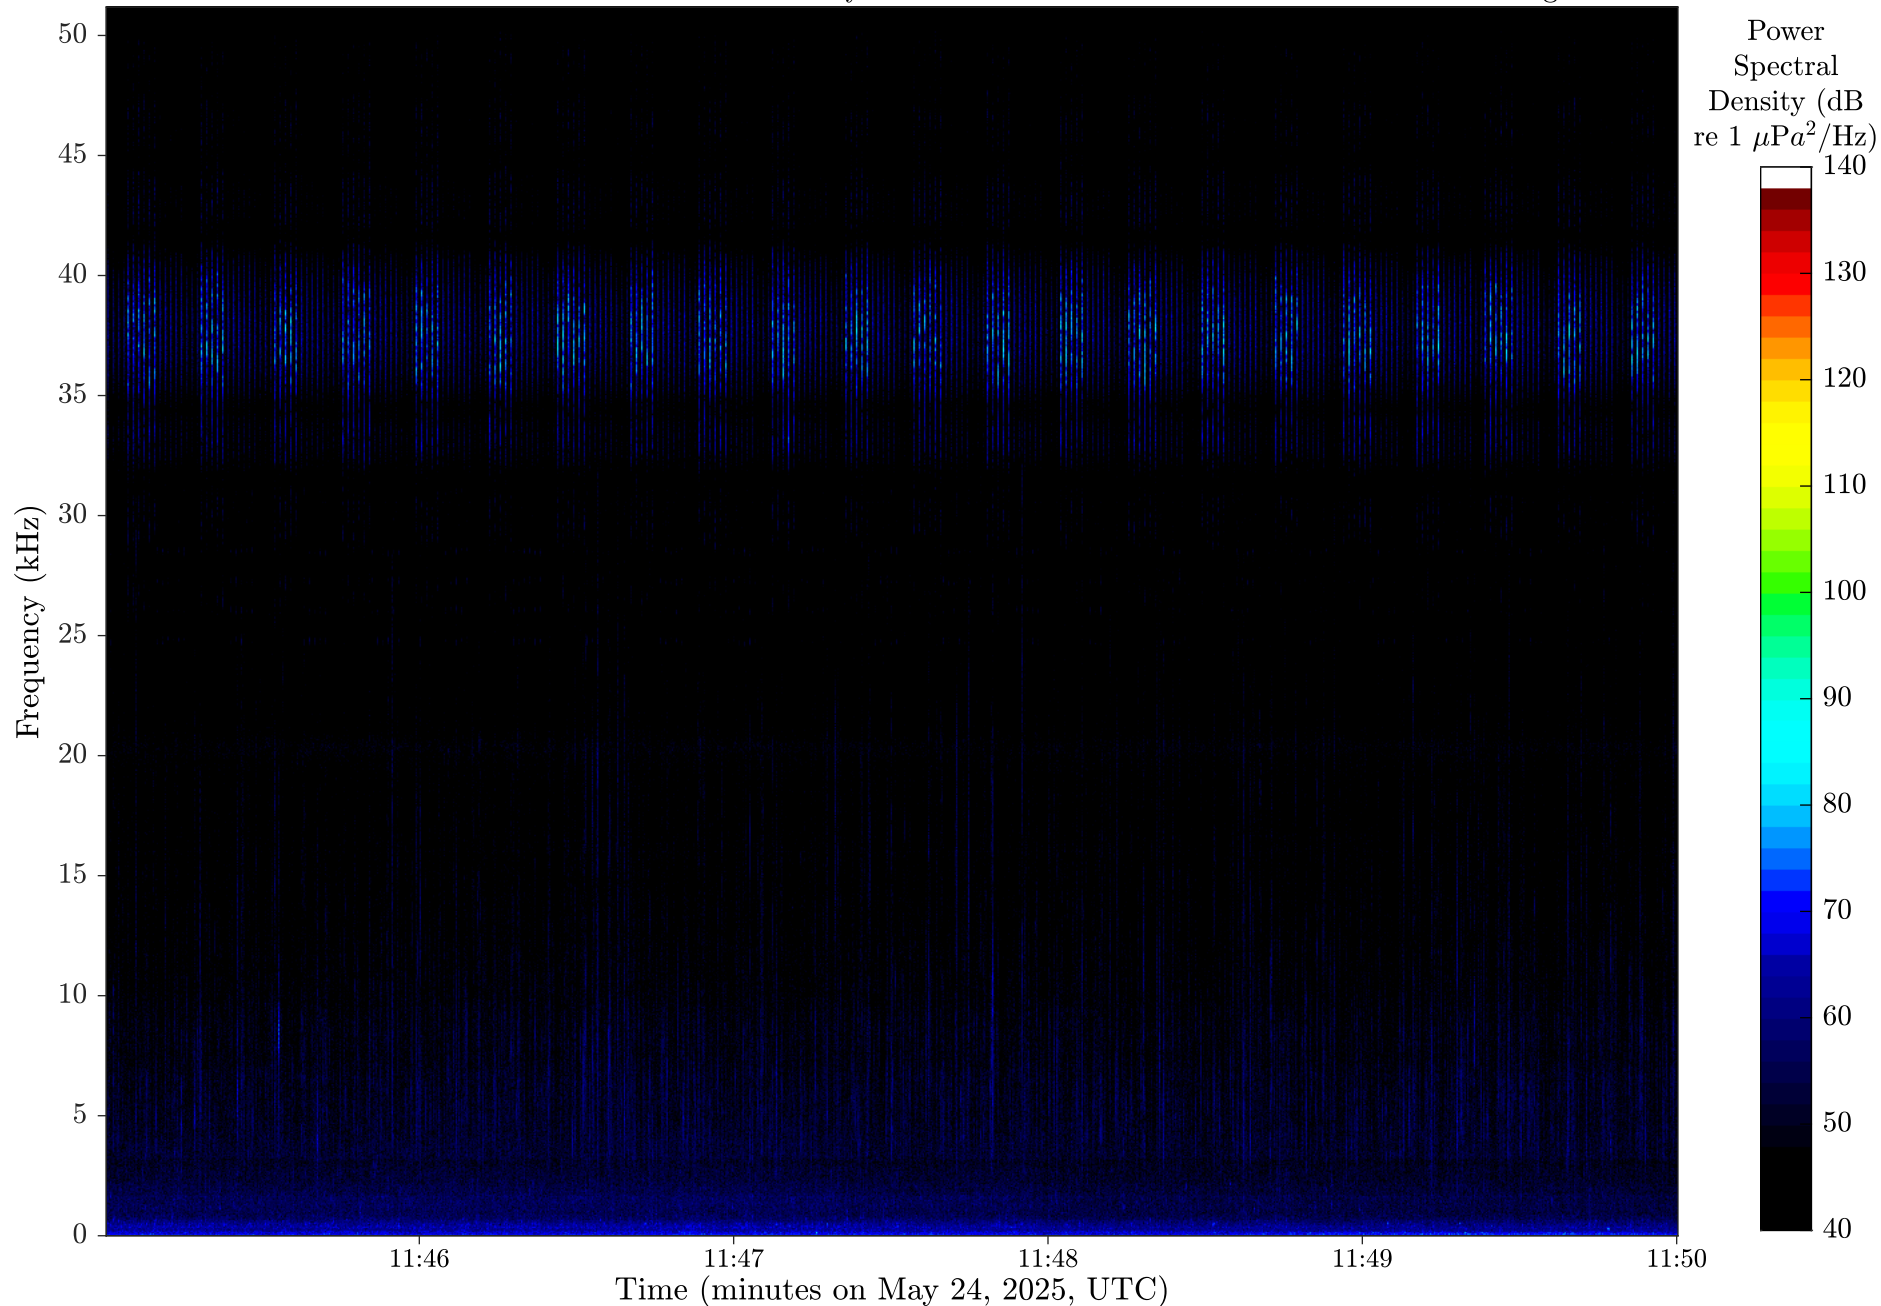


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:43 UTC

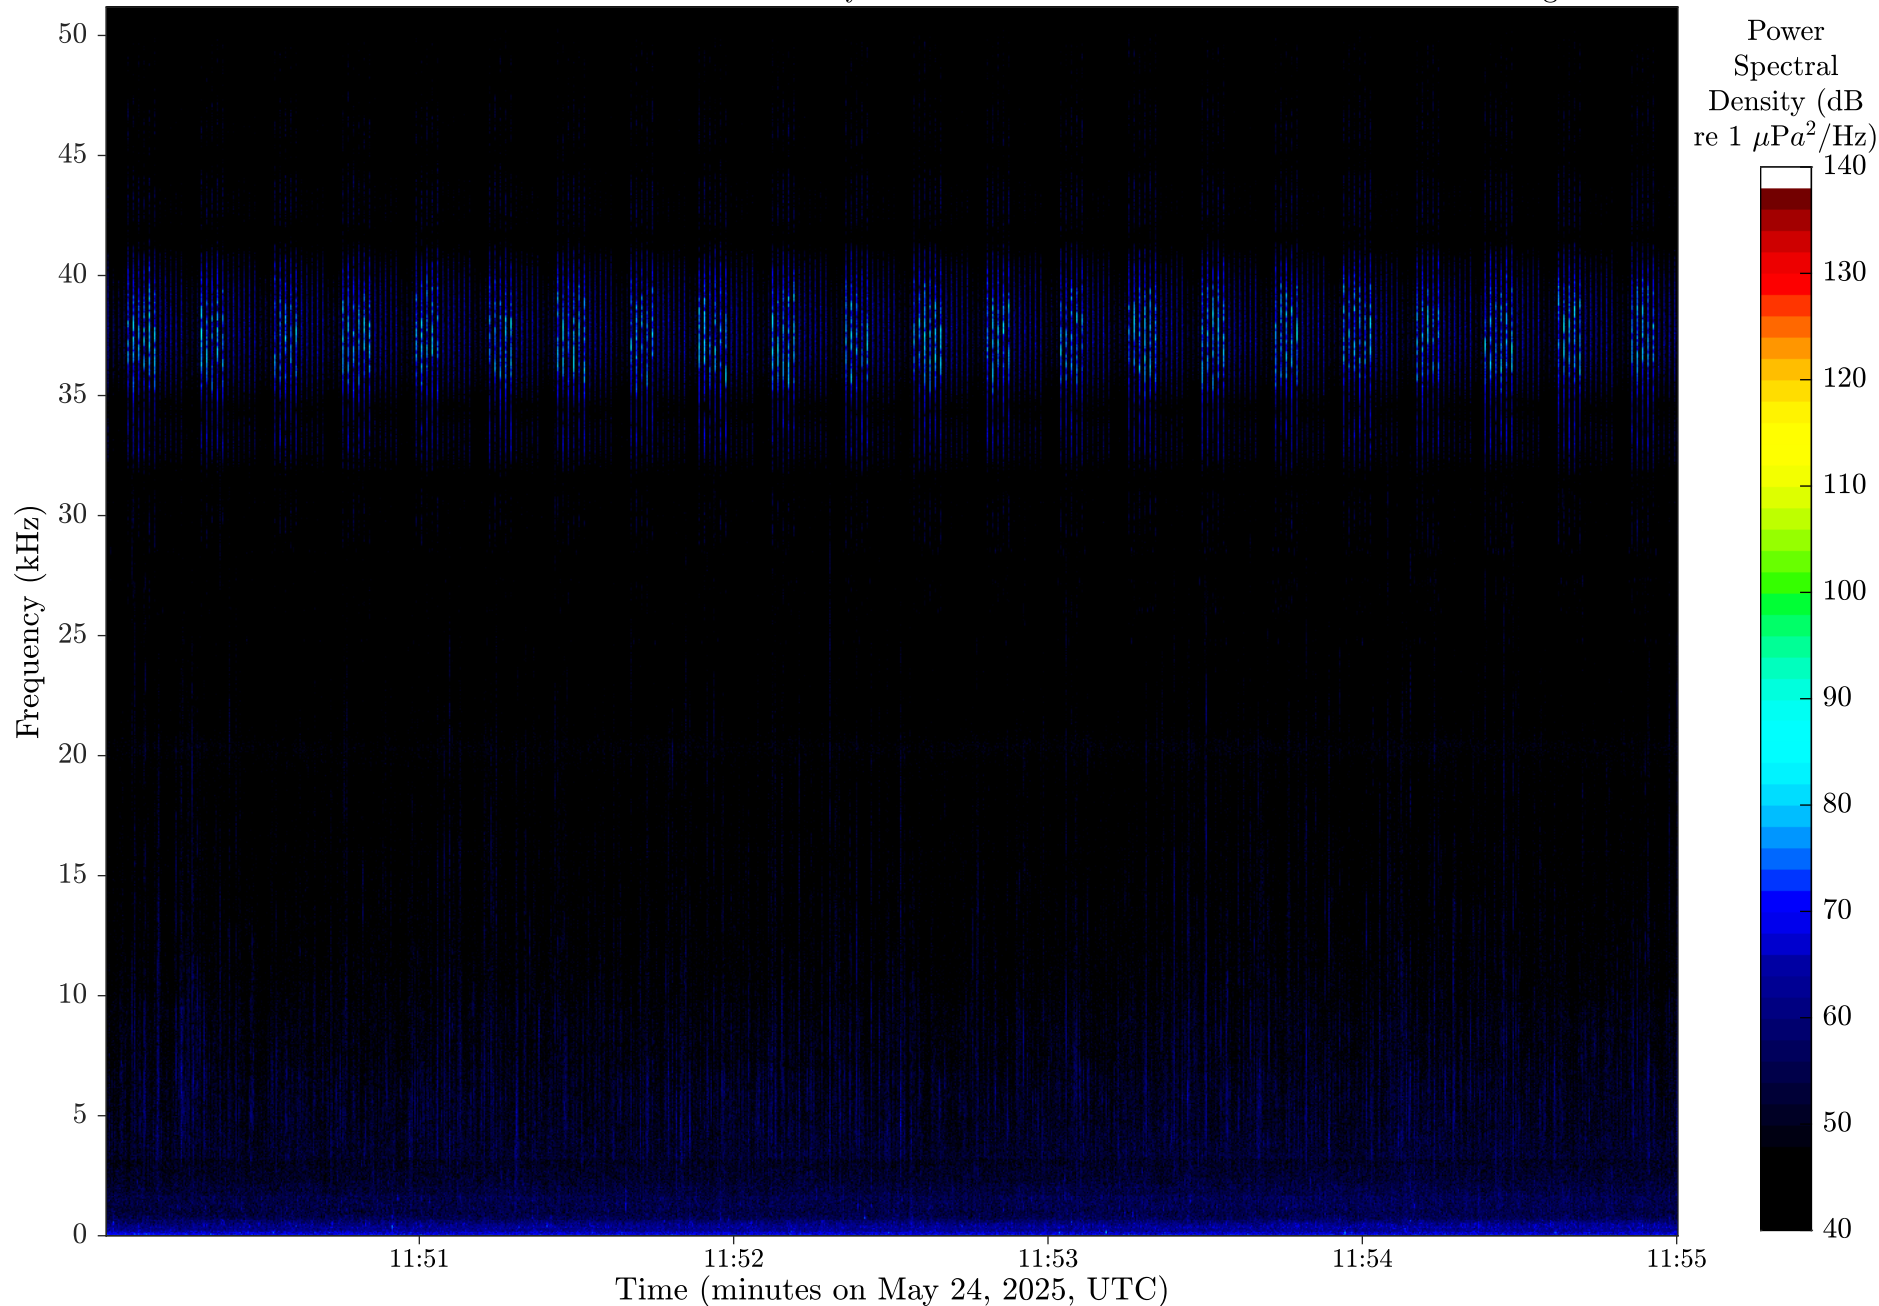


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:52 UTC

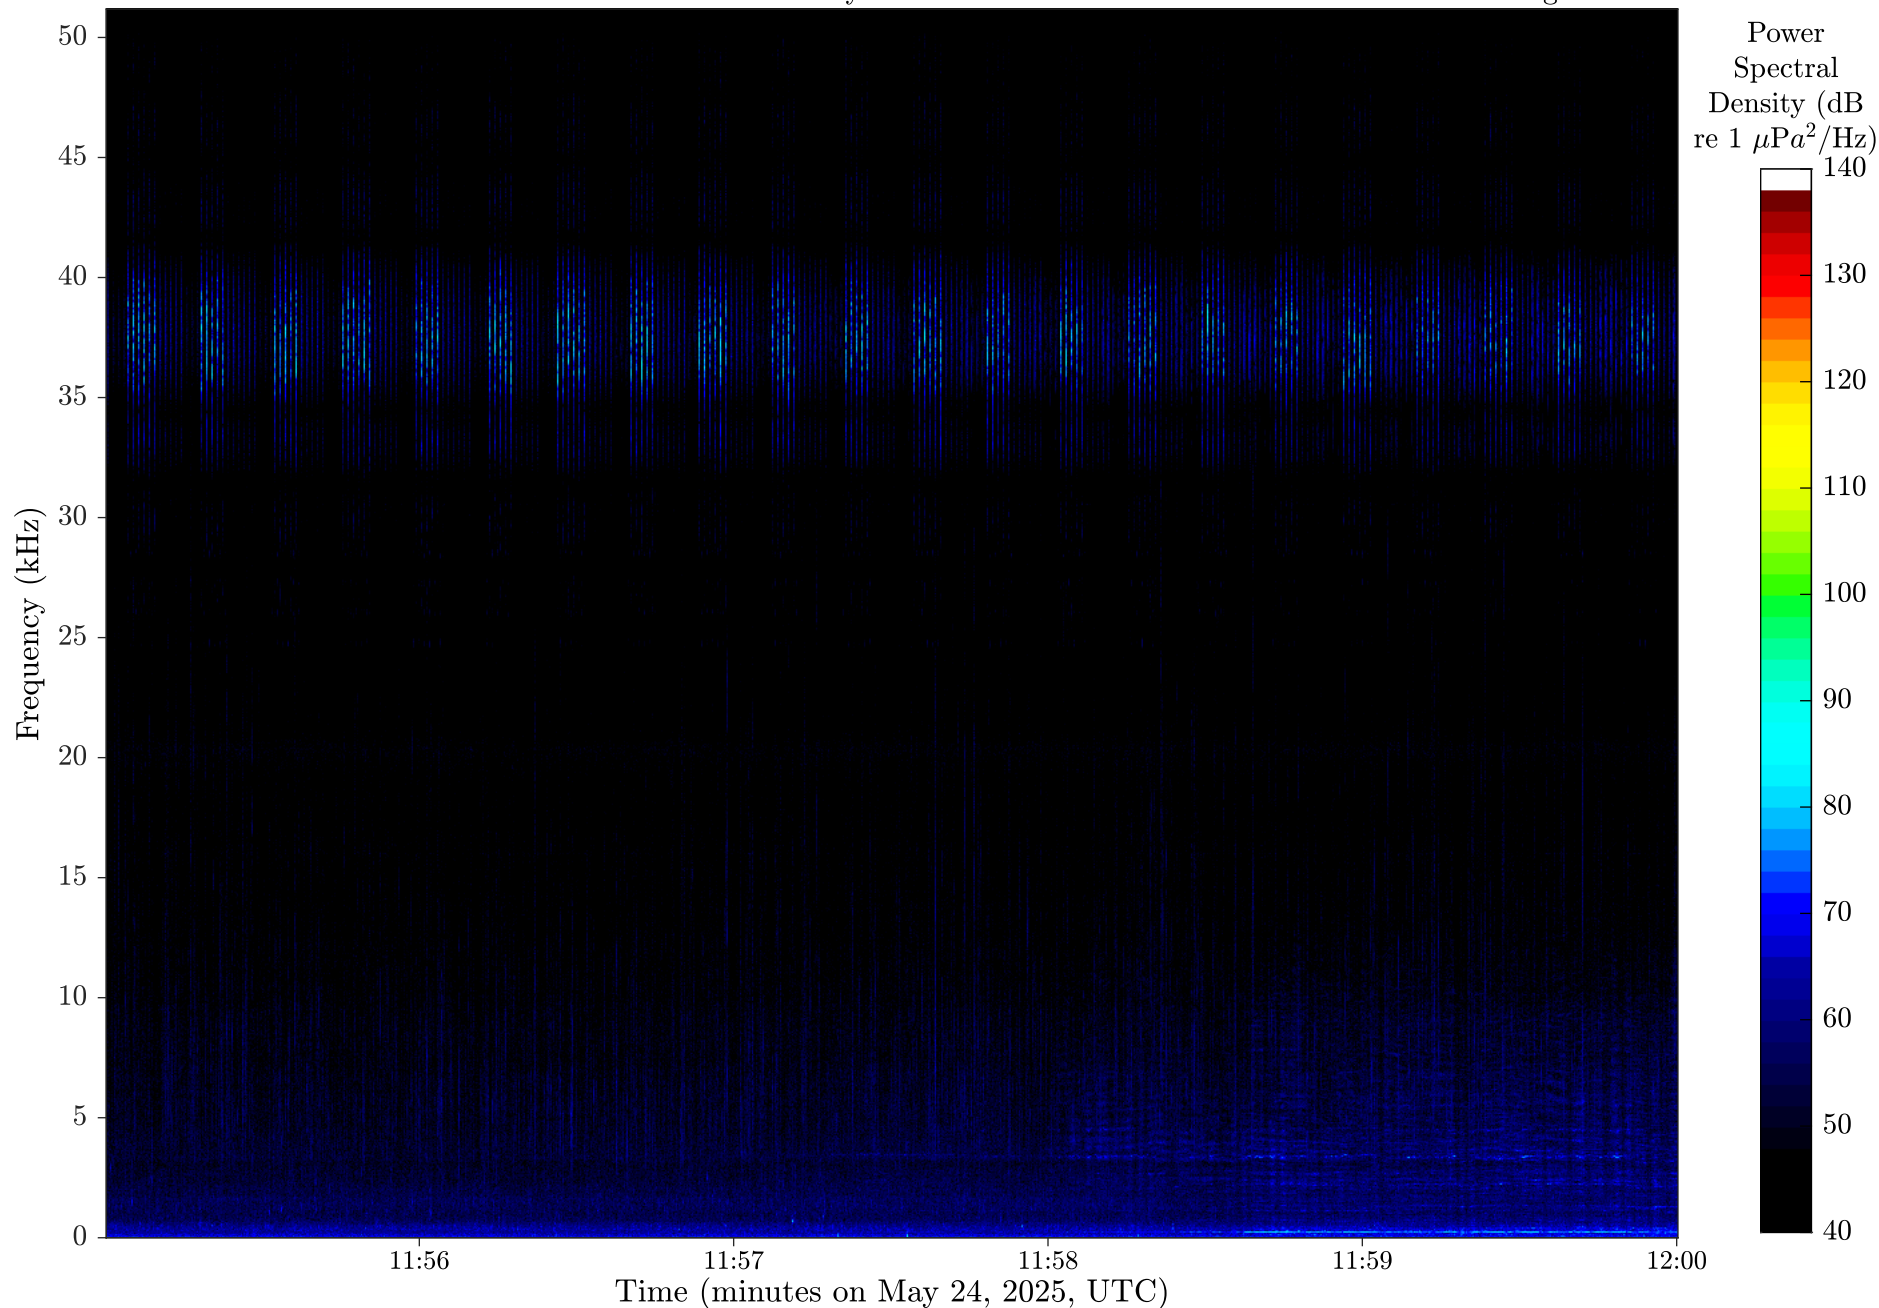


Comments: 31 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:00 UTC

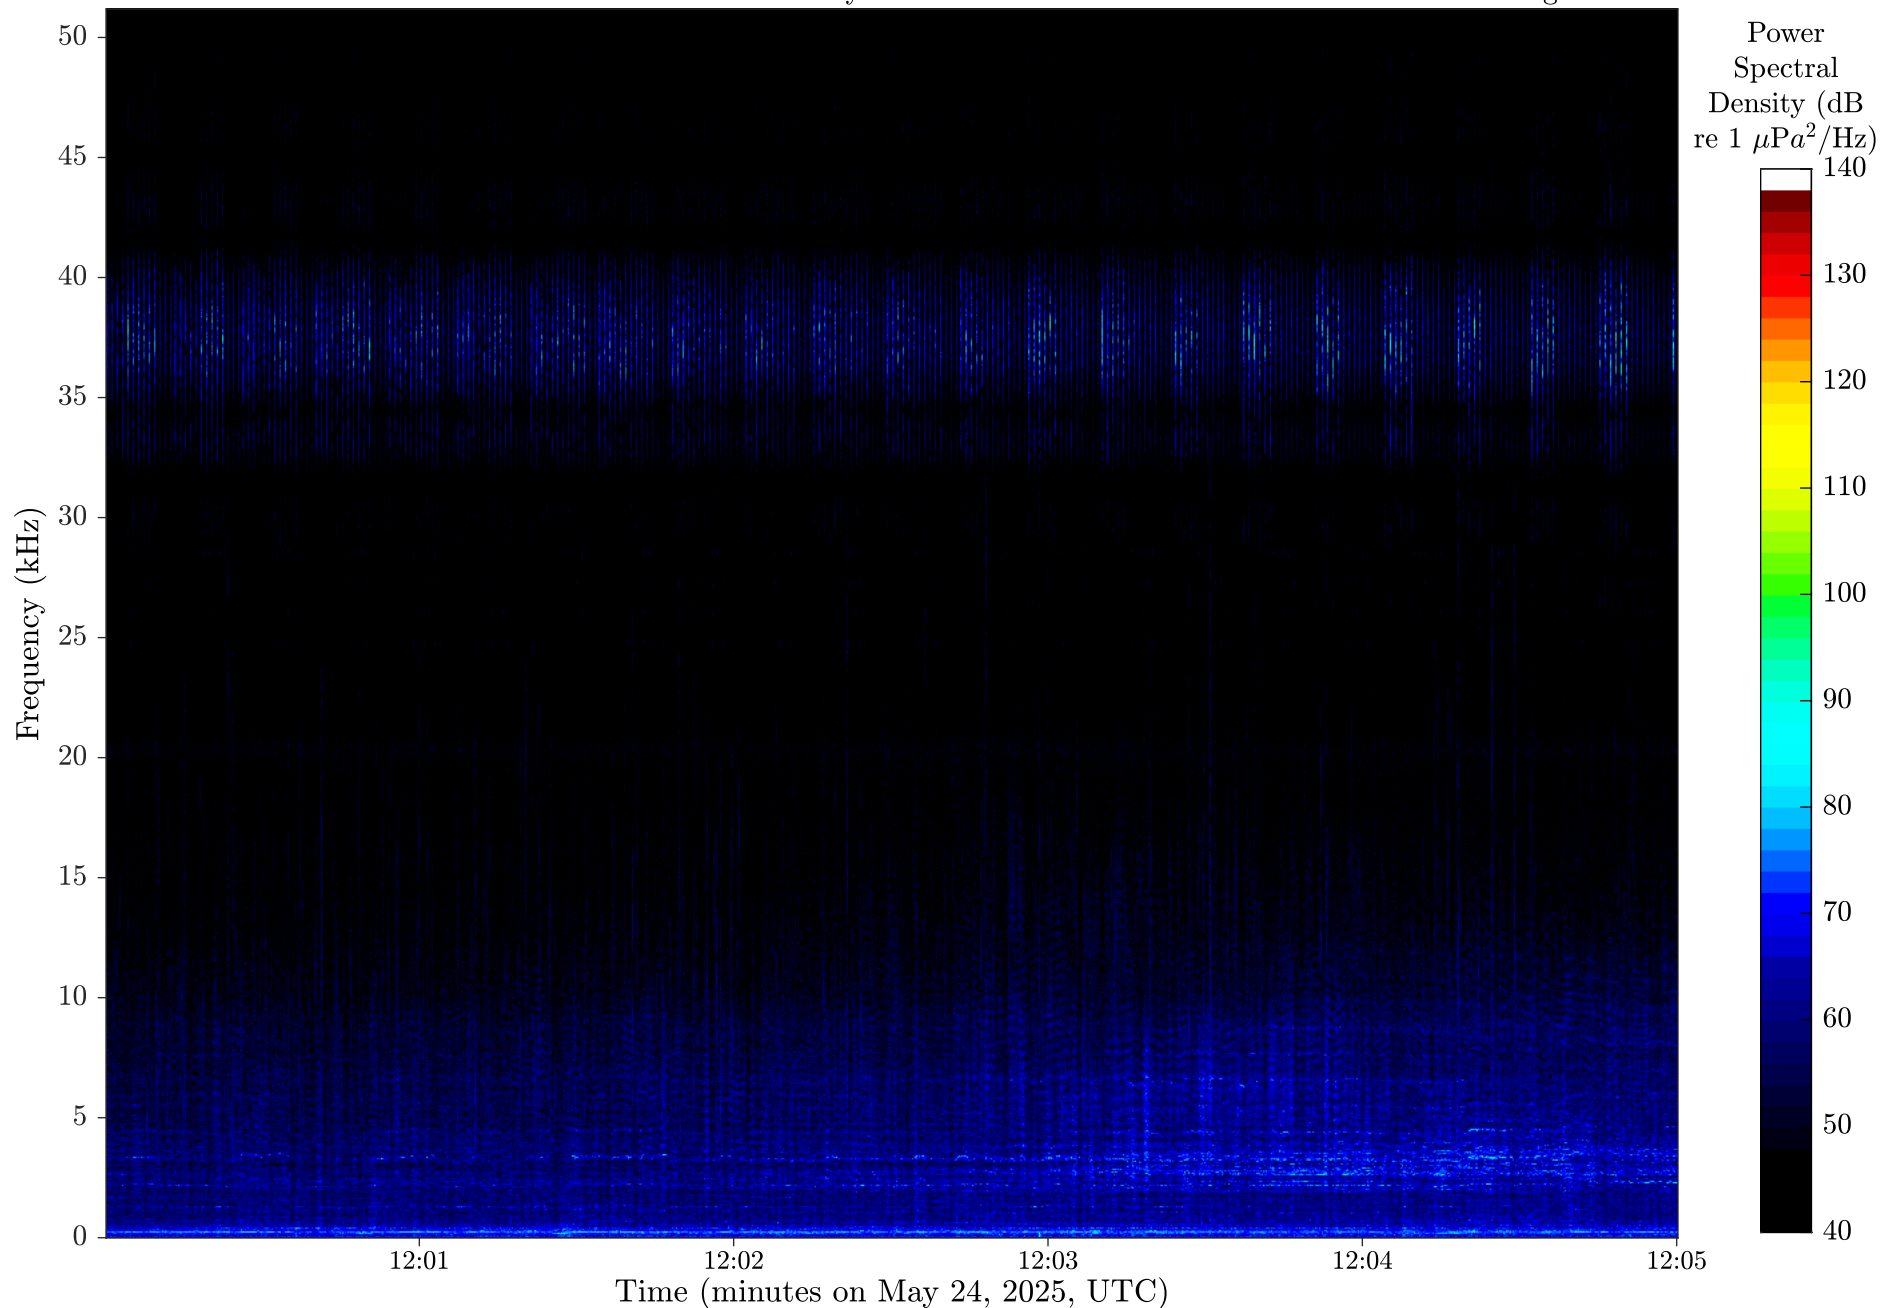


Comments: 28.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:09 UTC

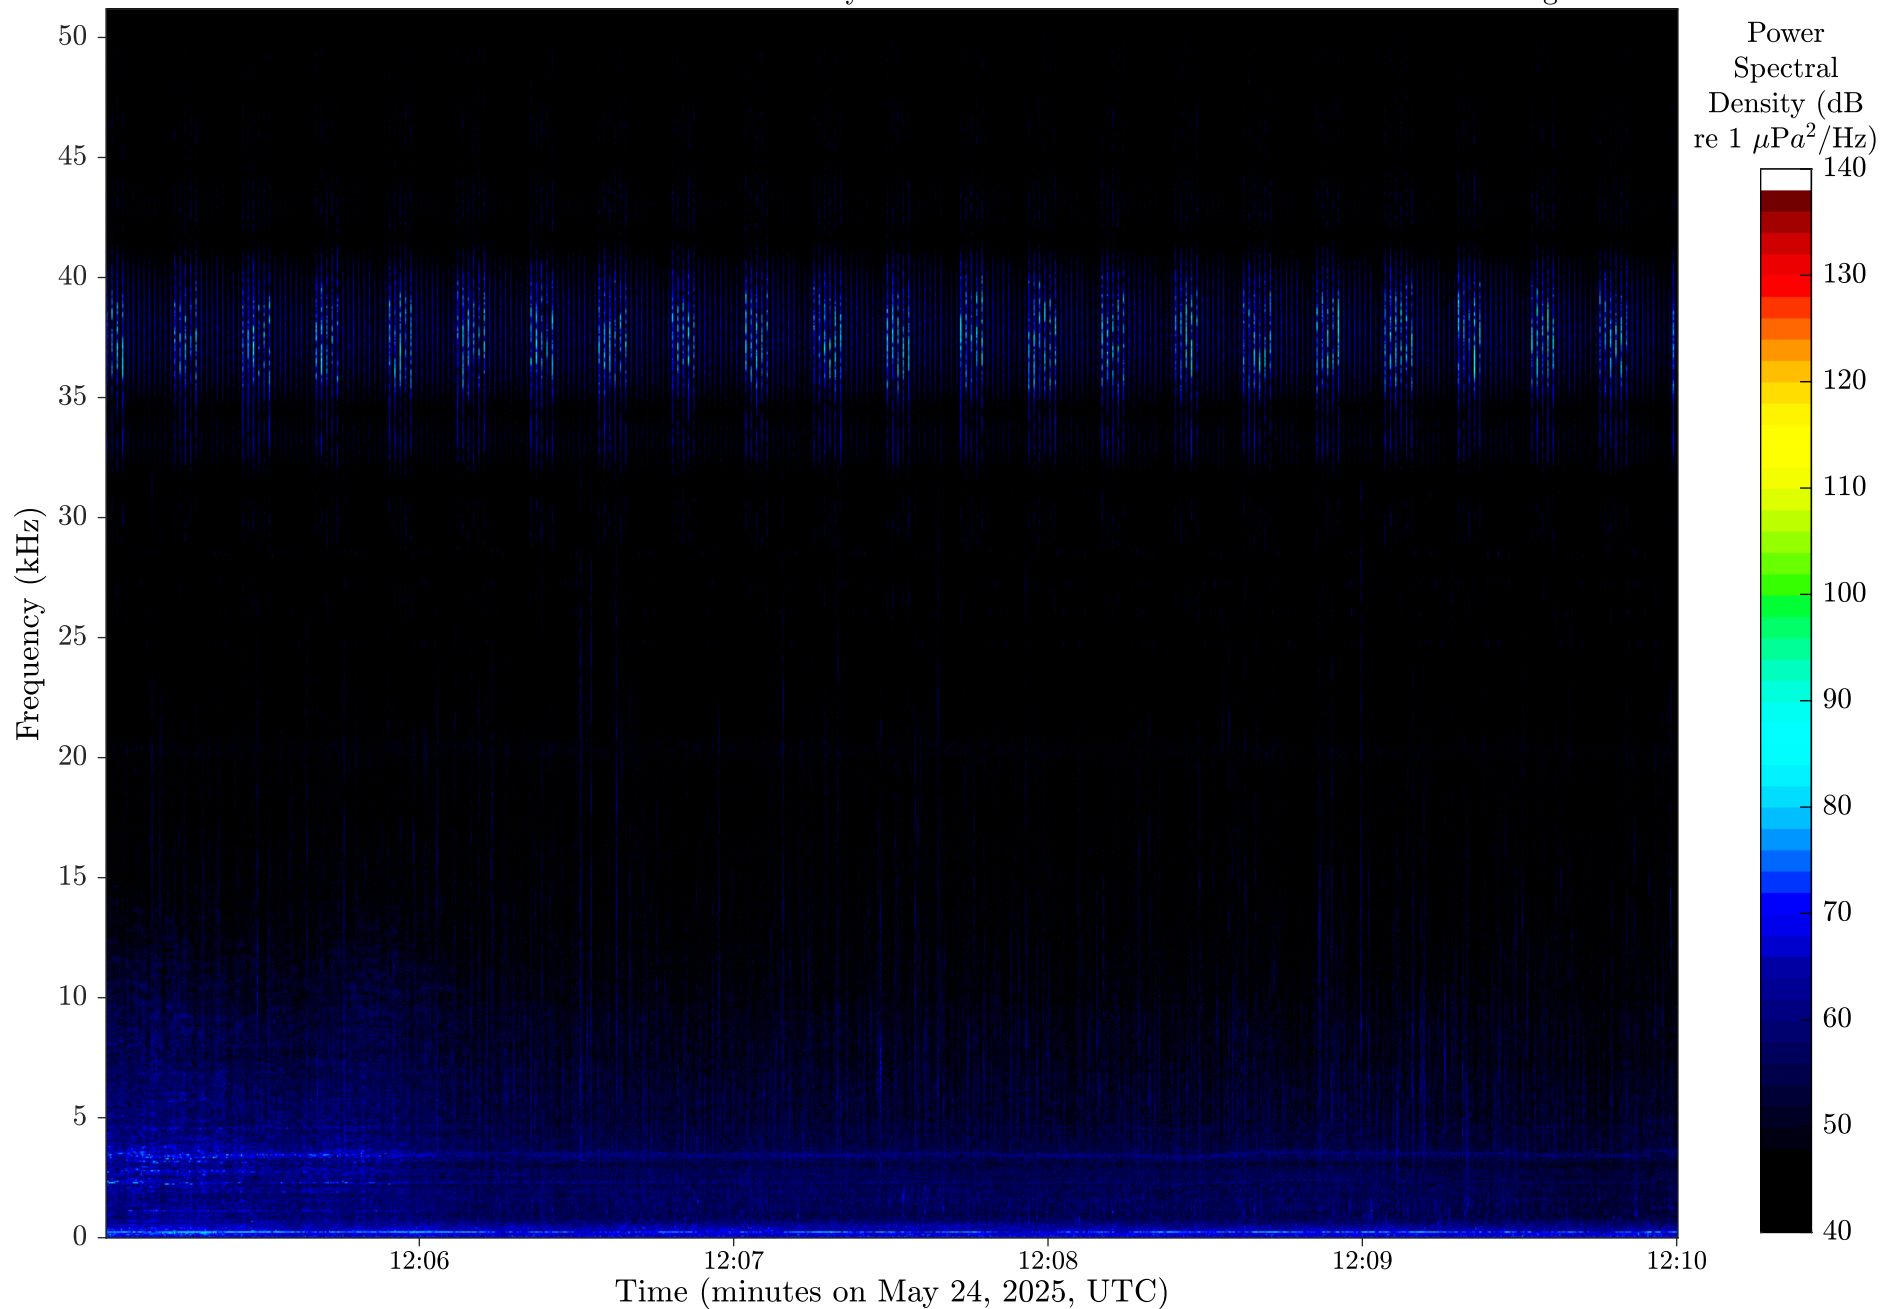


Comments: 29.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:17 UTC

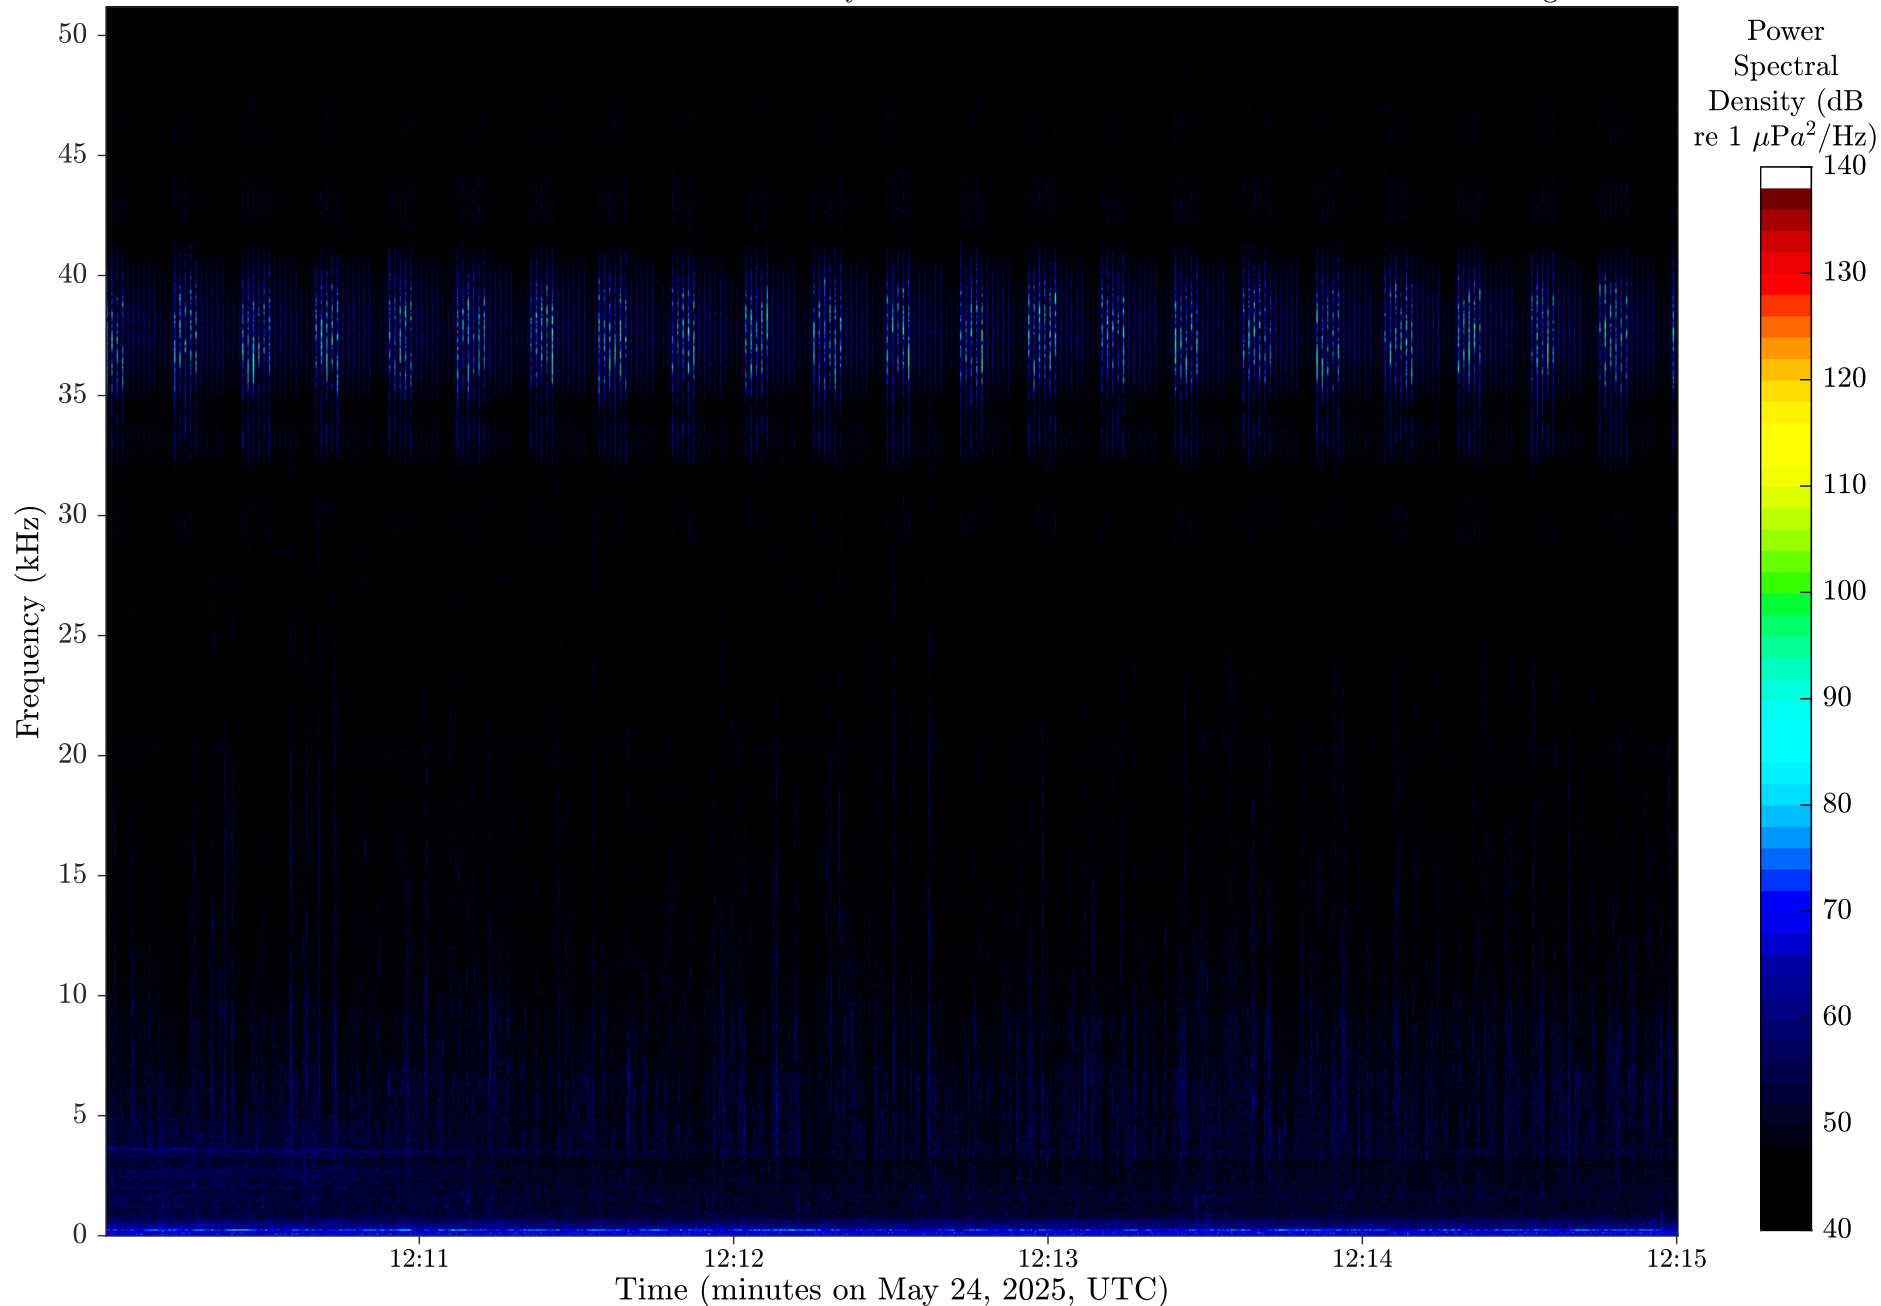


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:26 UTC

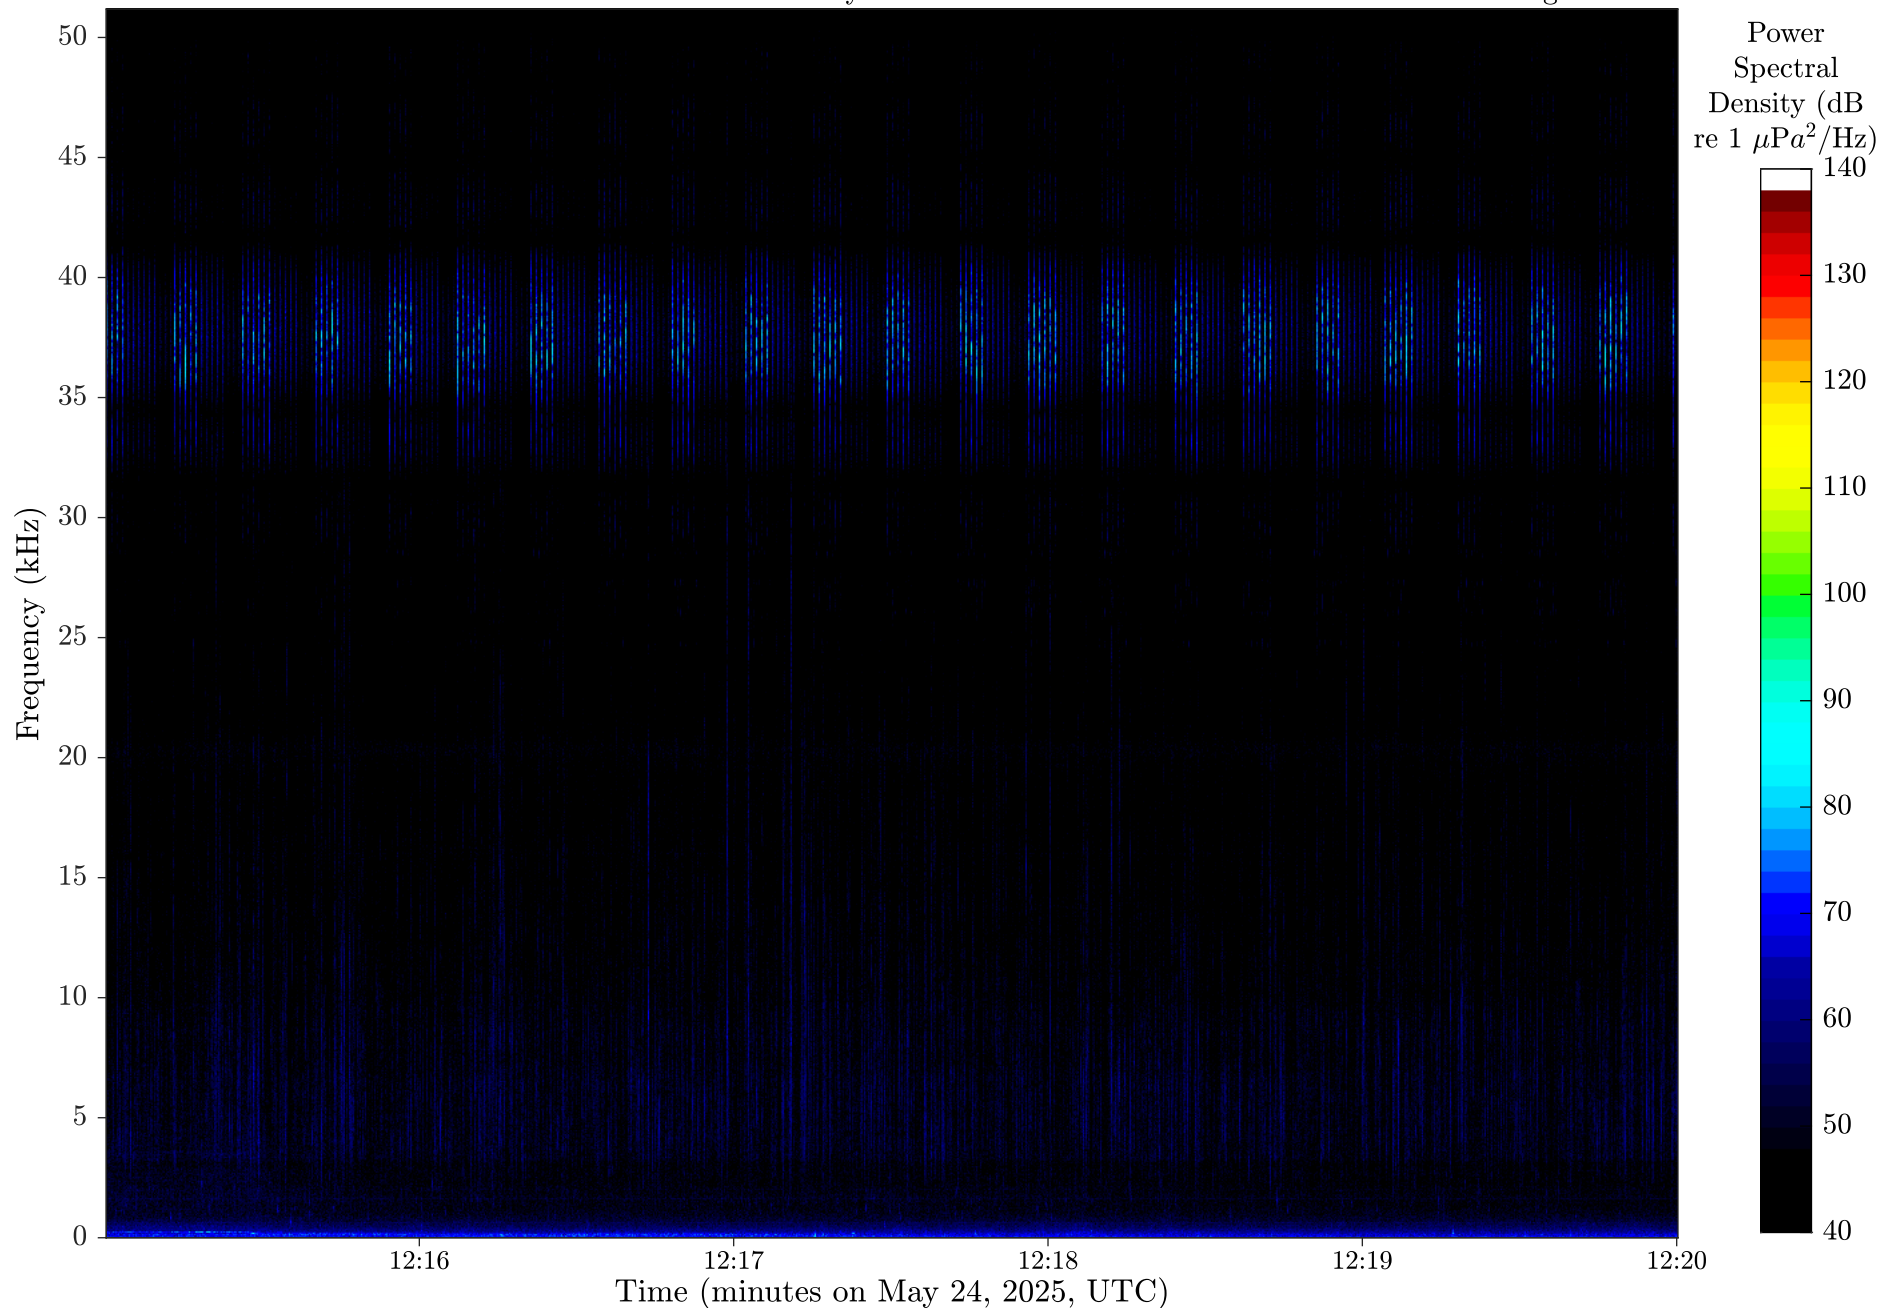


Comments: 32.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:34 UTC

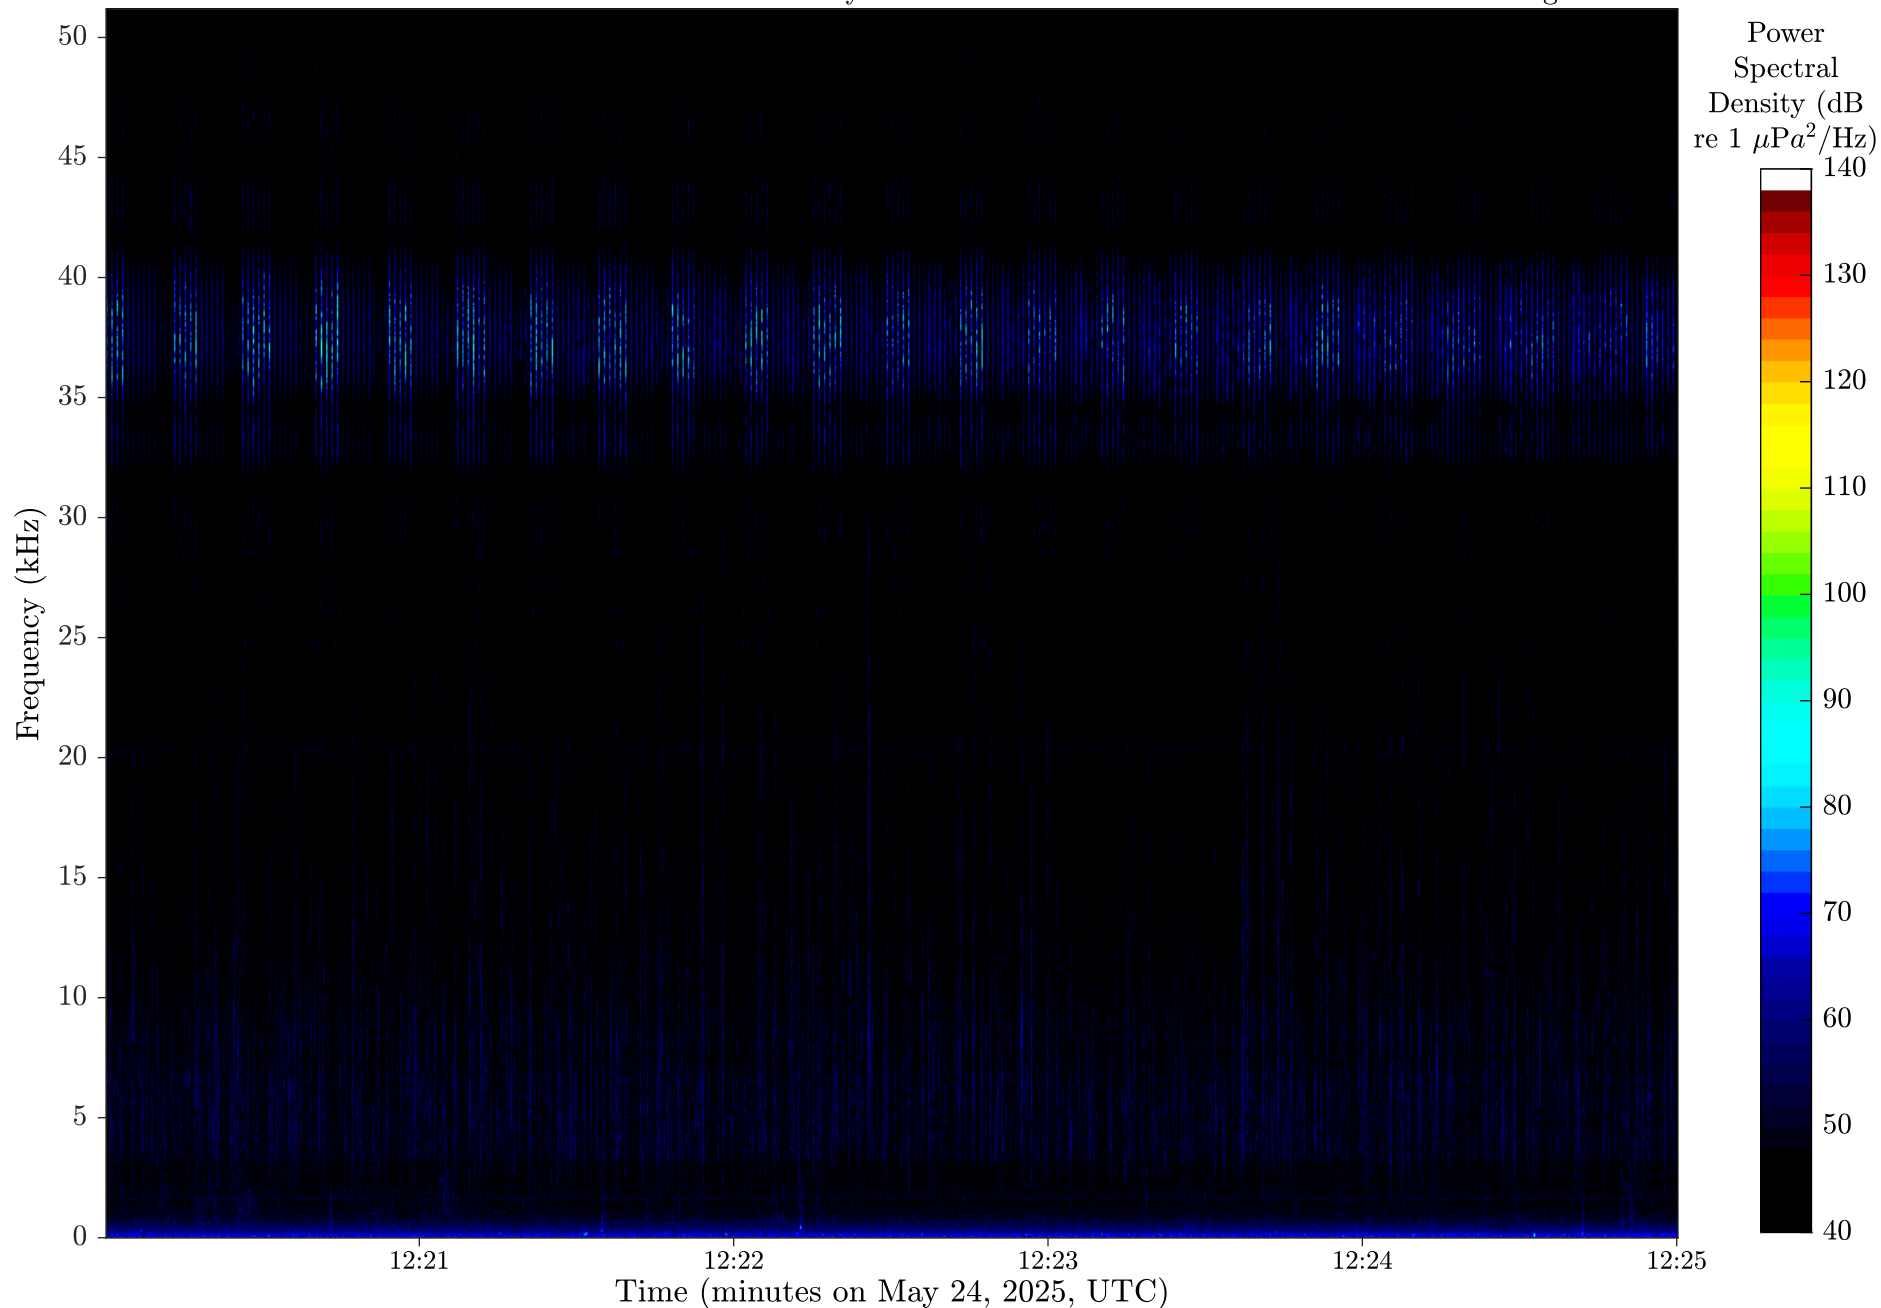


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:42 UTC

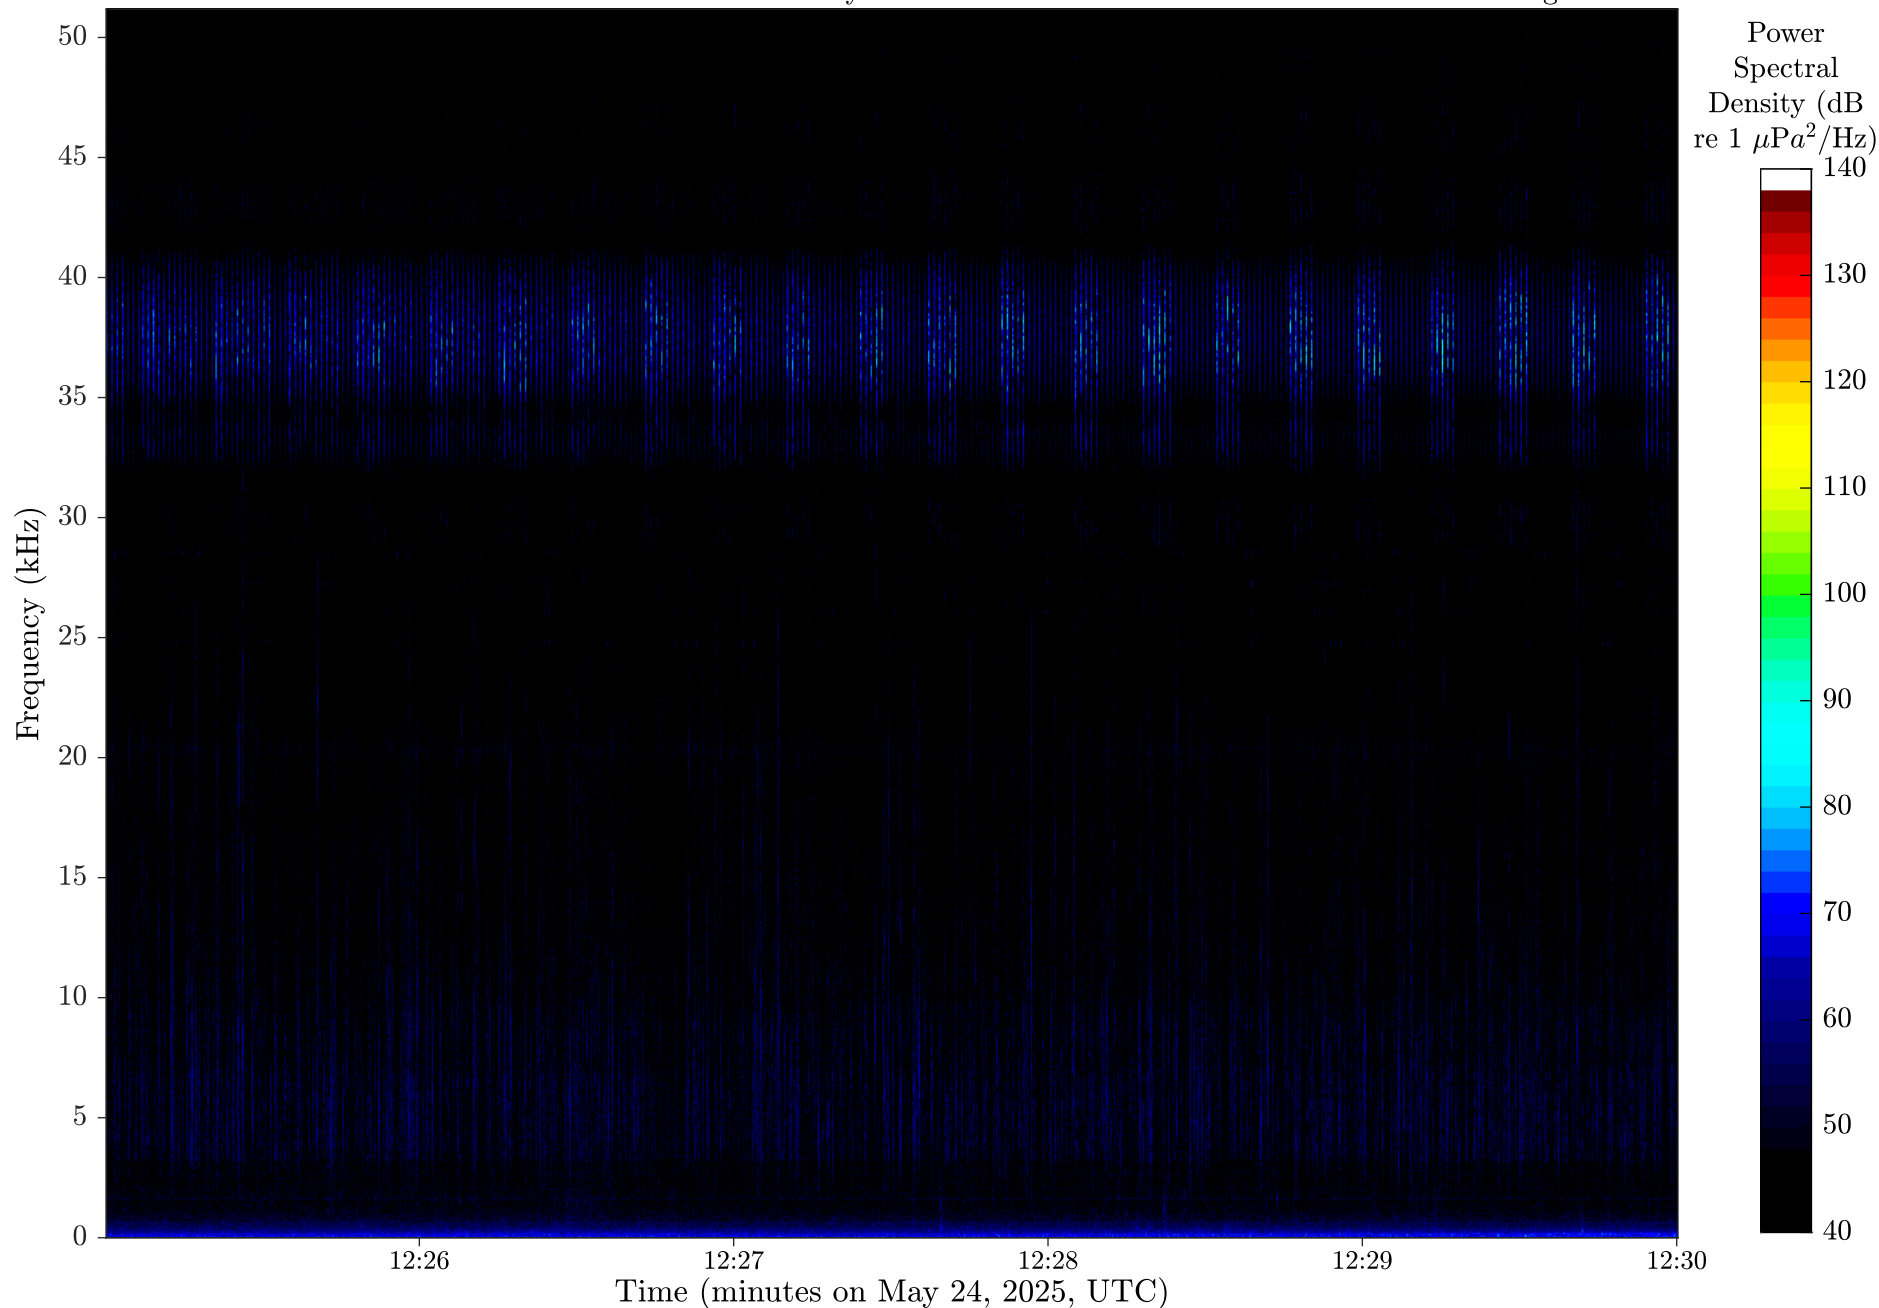


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:51 UTC

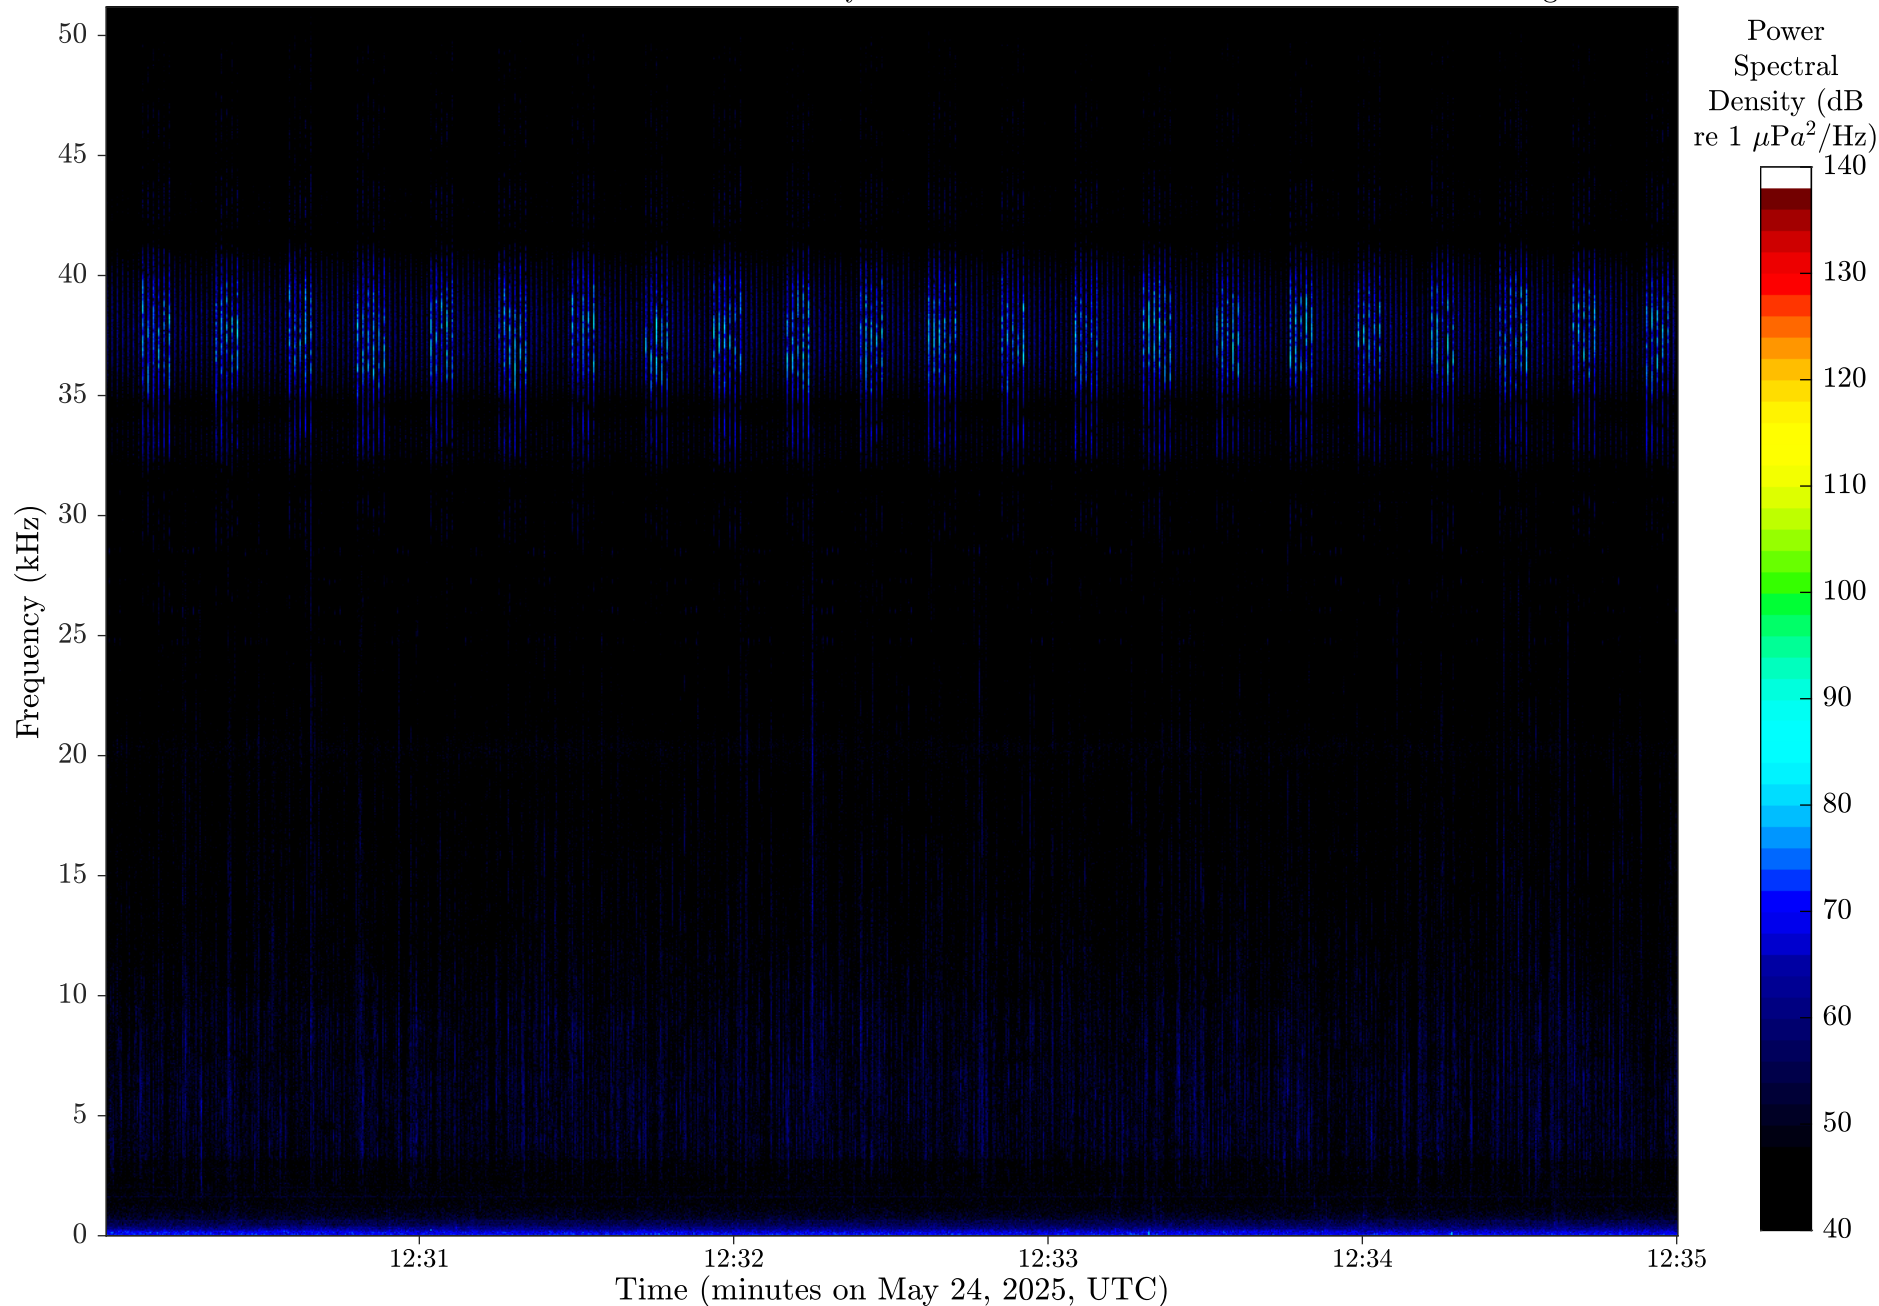


Comments: 31.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:59 UTC

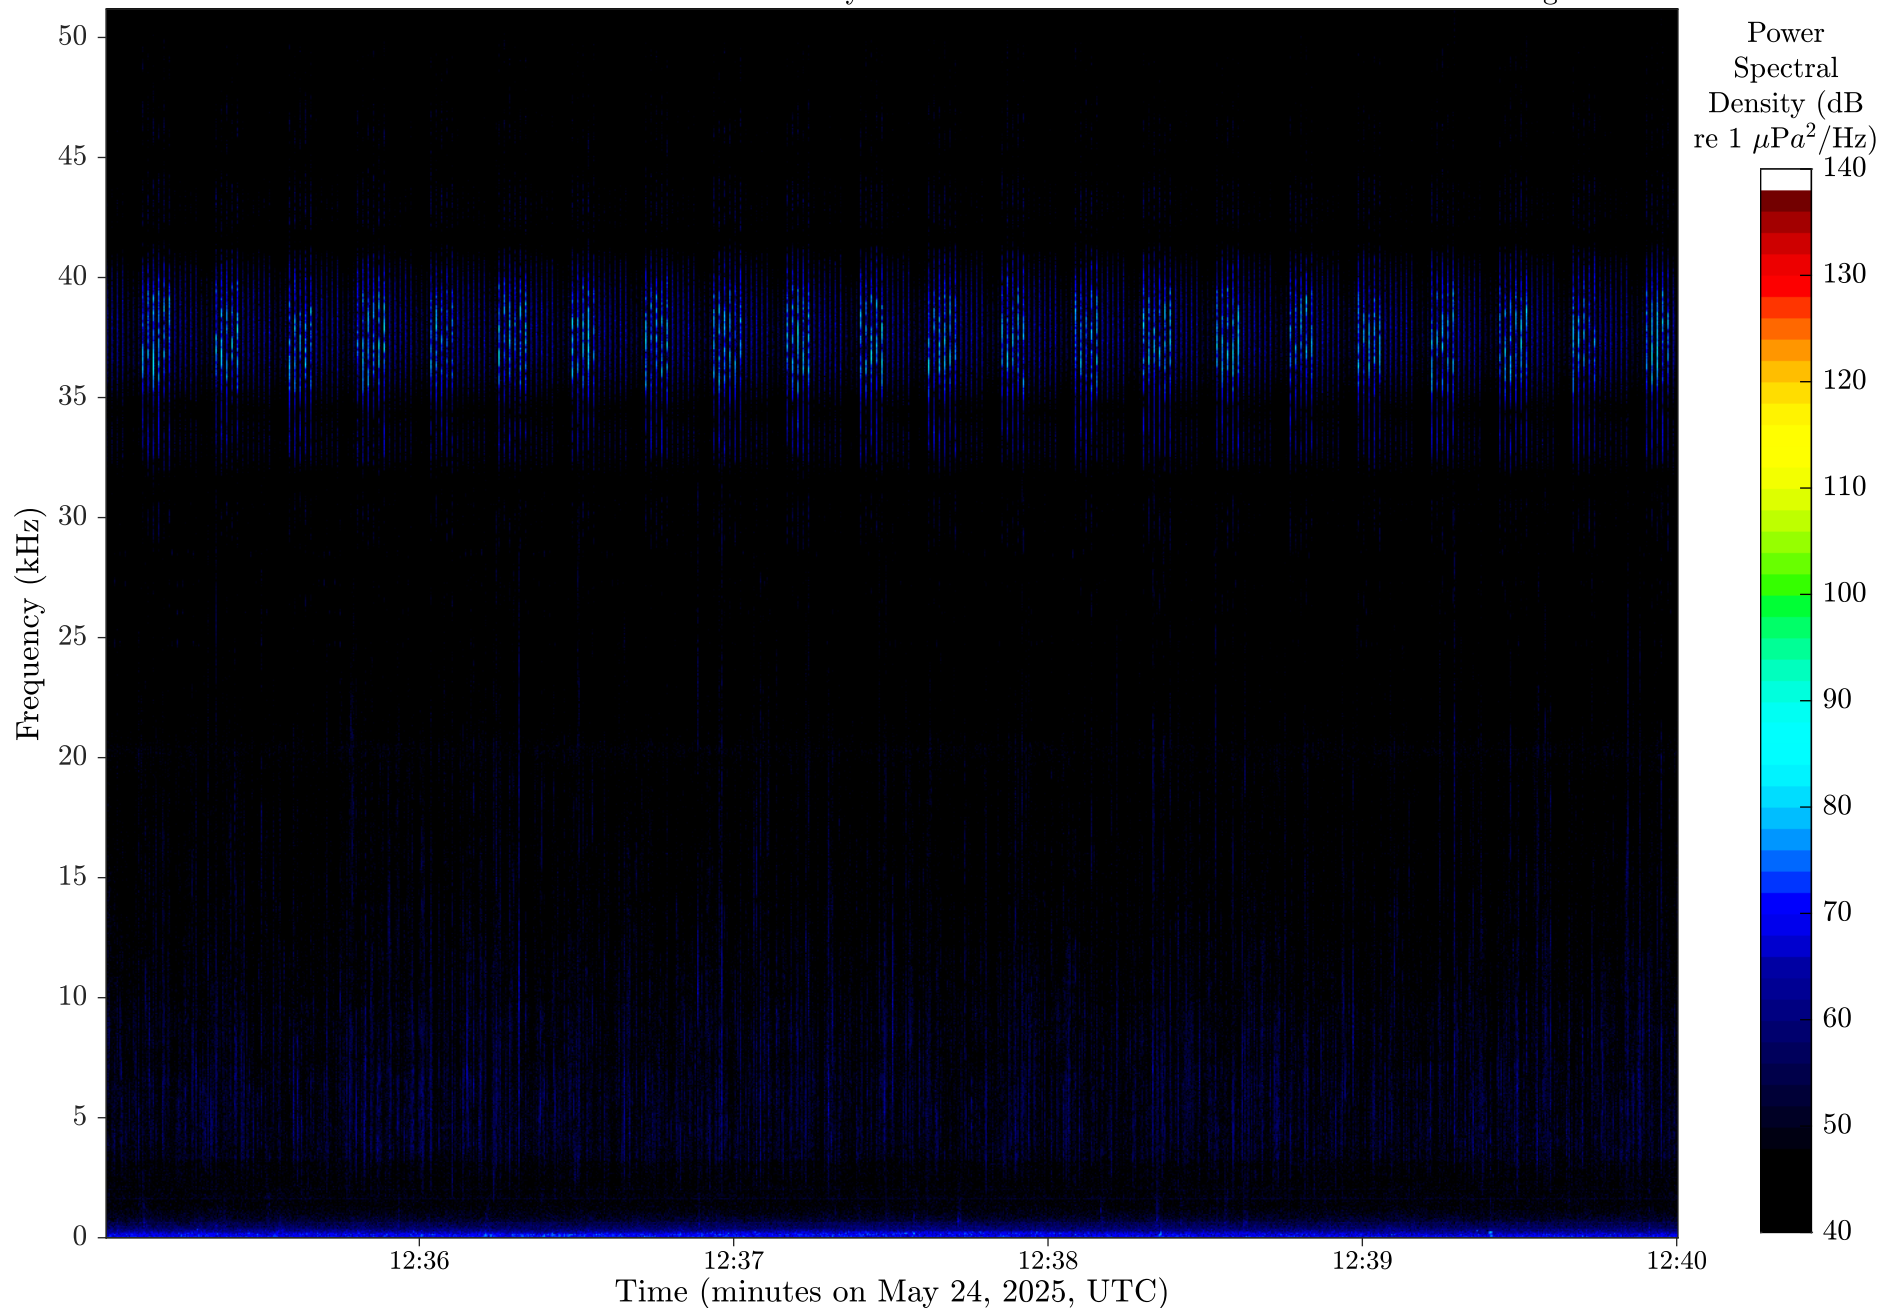


Comments: 32.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:36:07 UTC

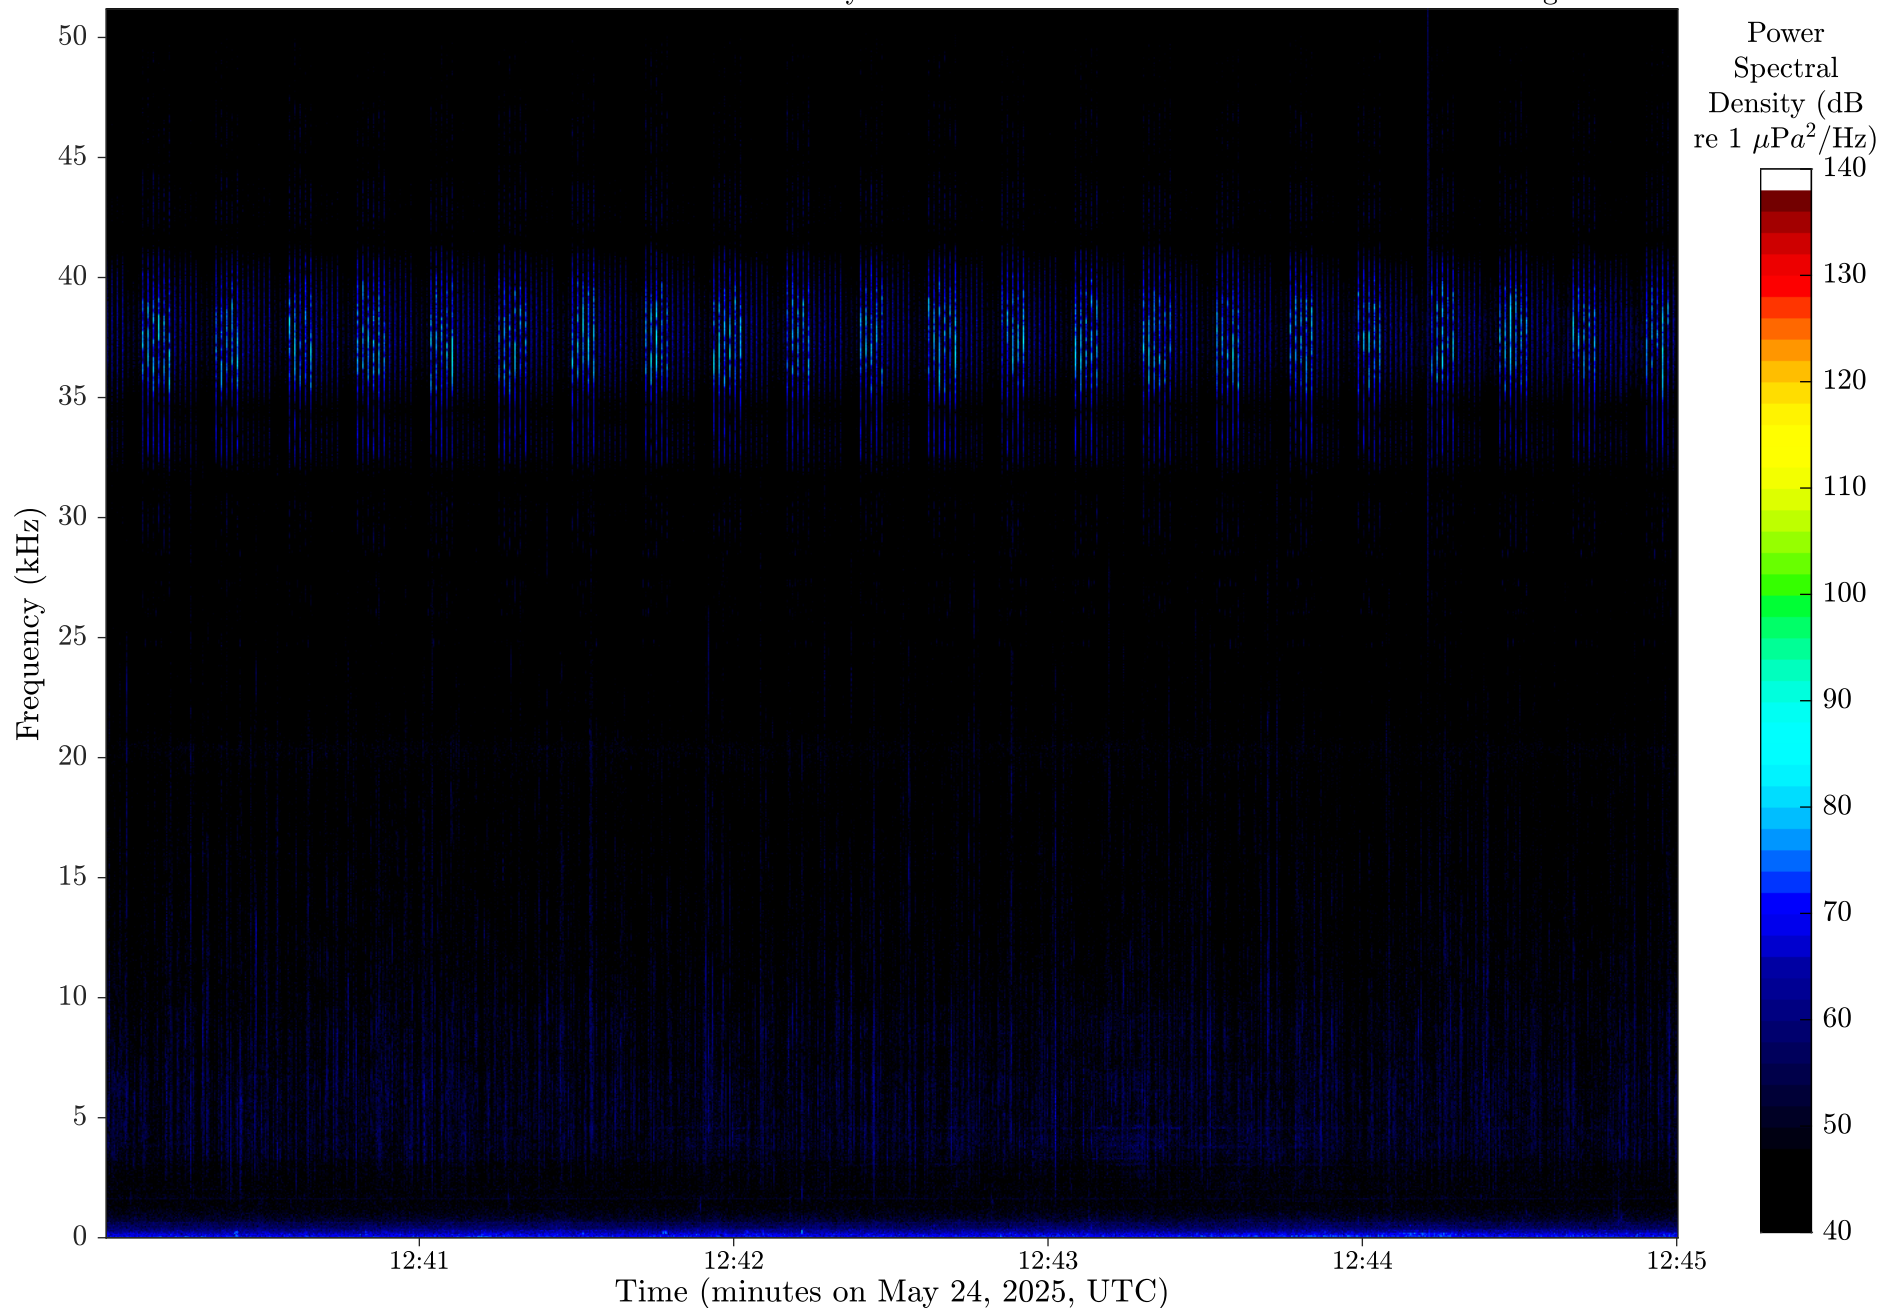


Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:15 UTC

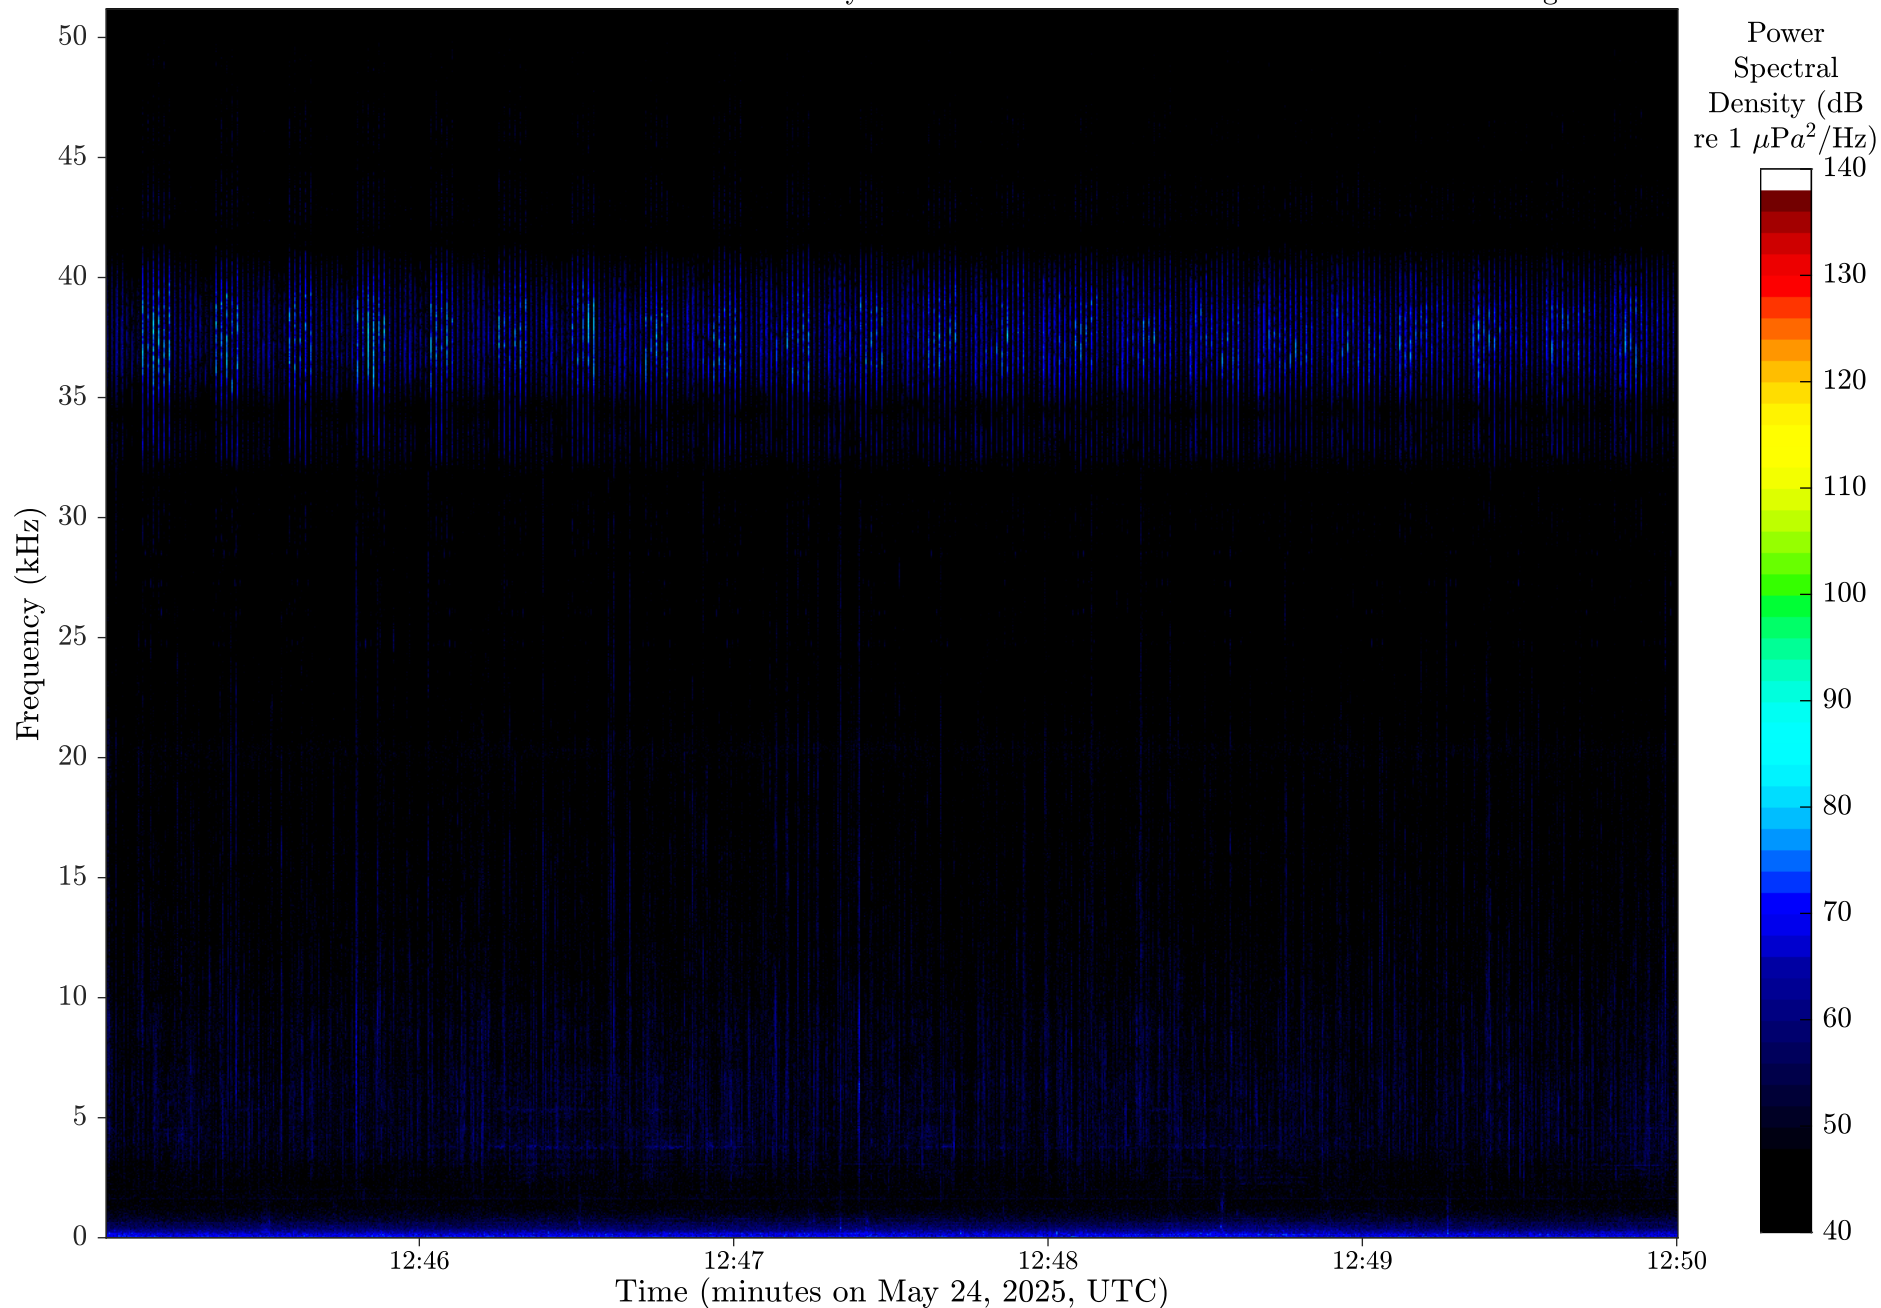


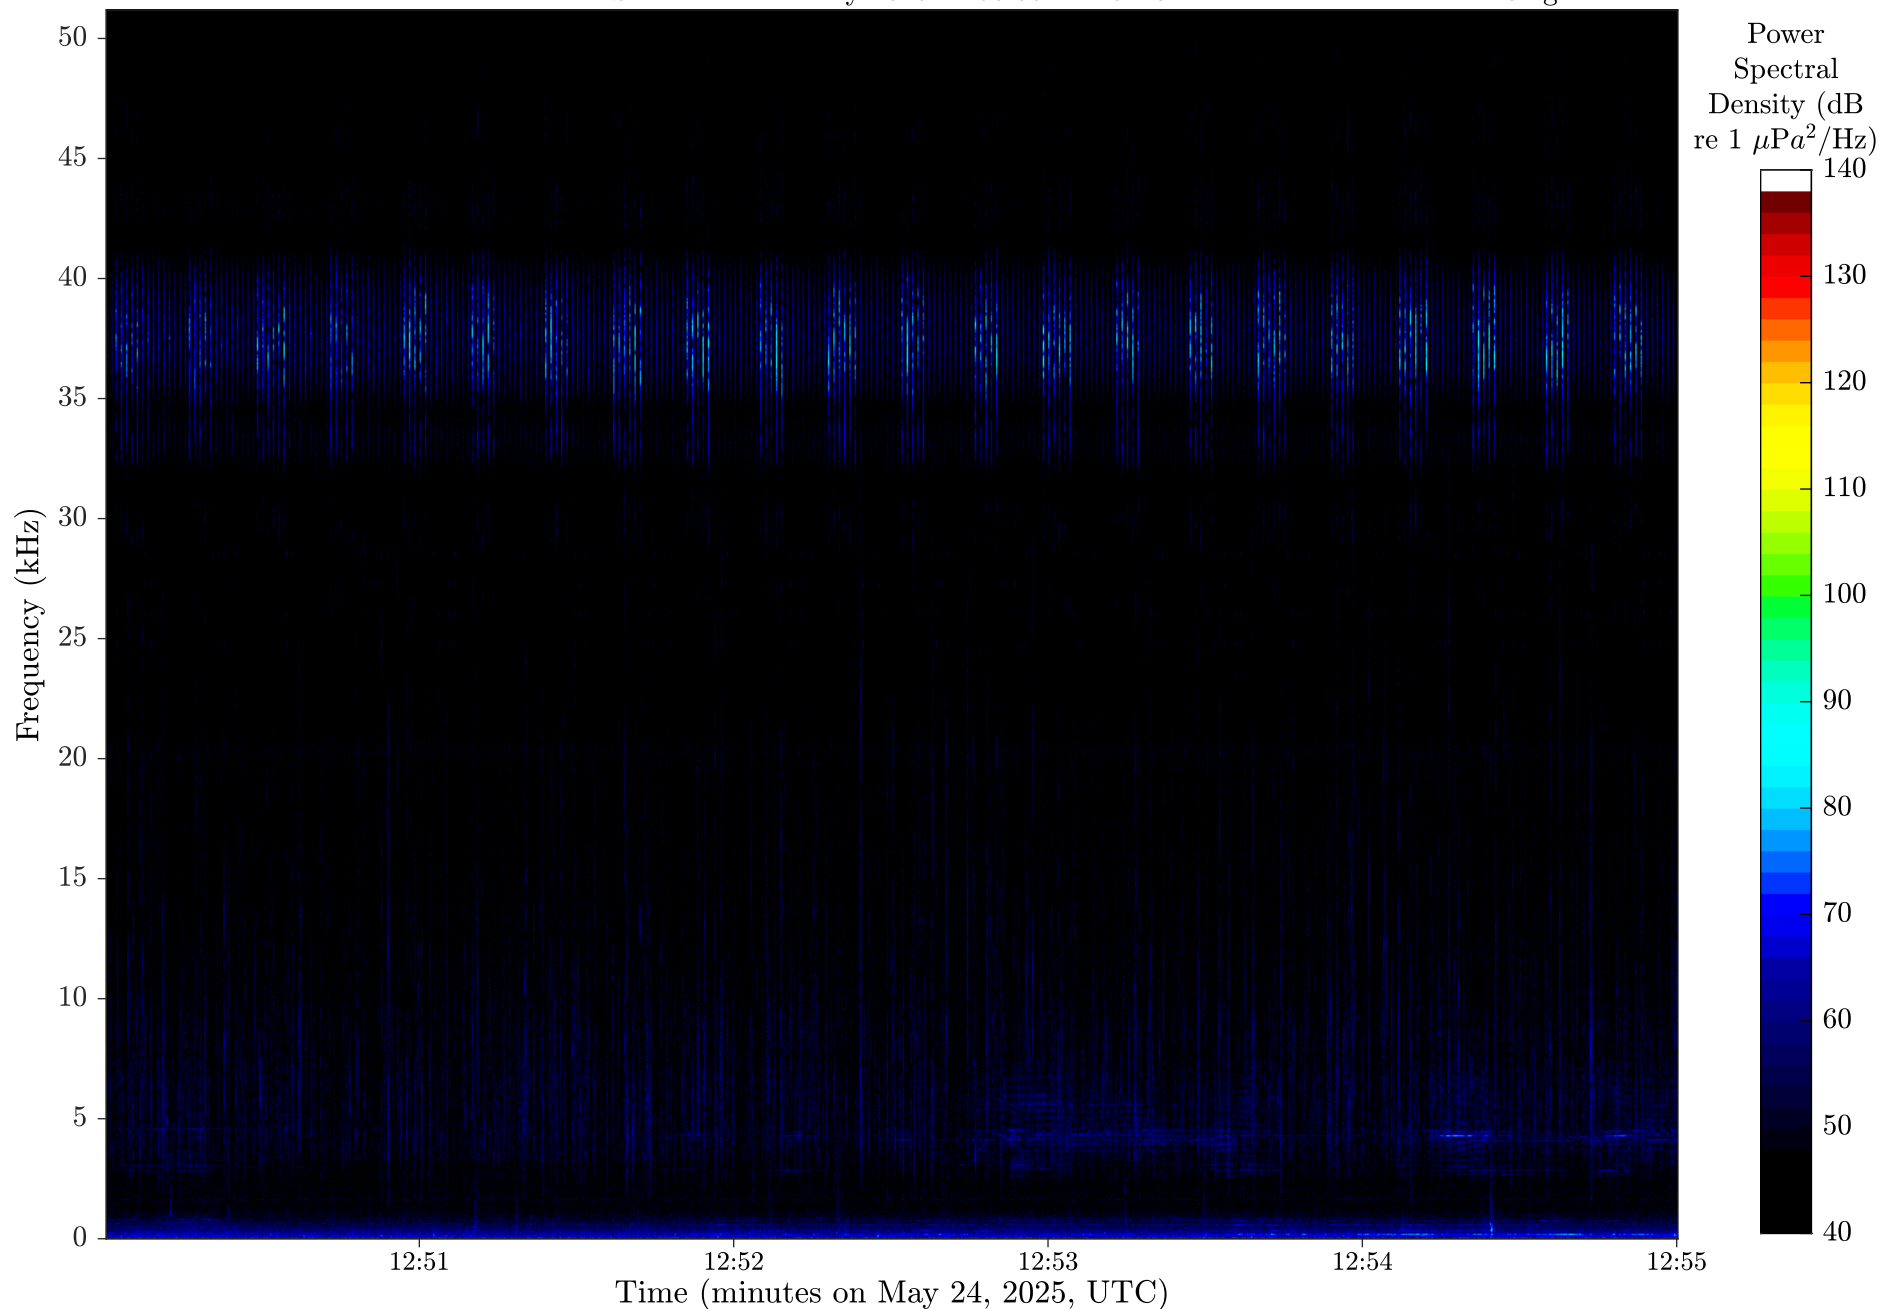

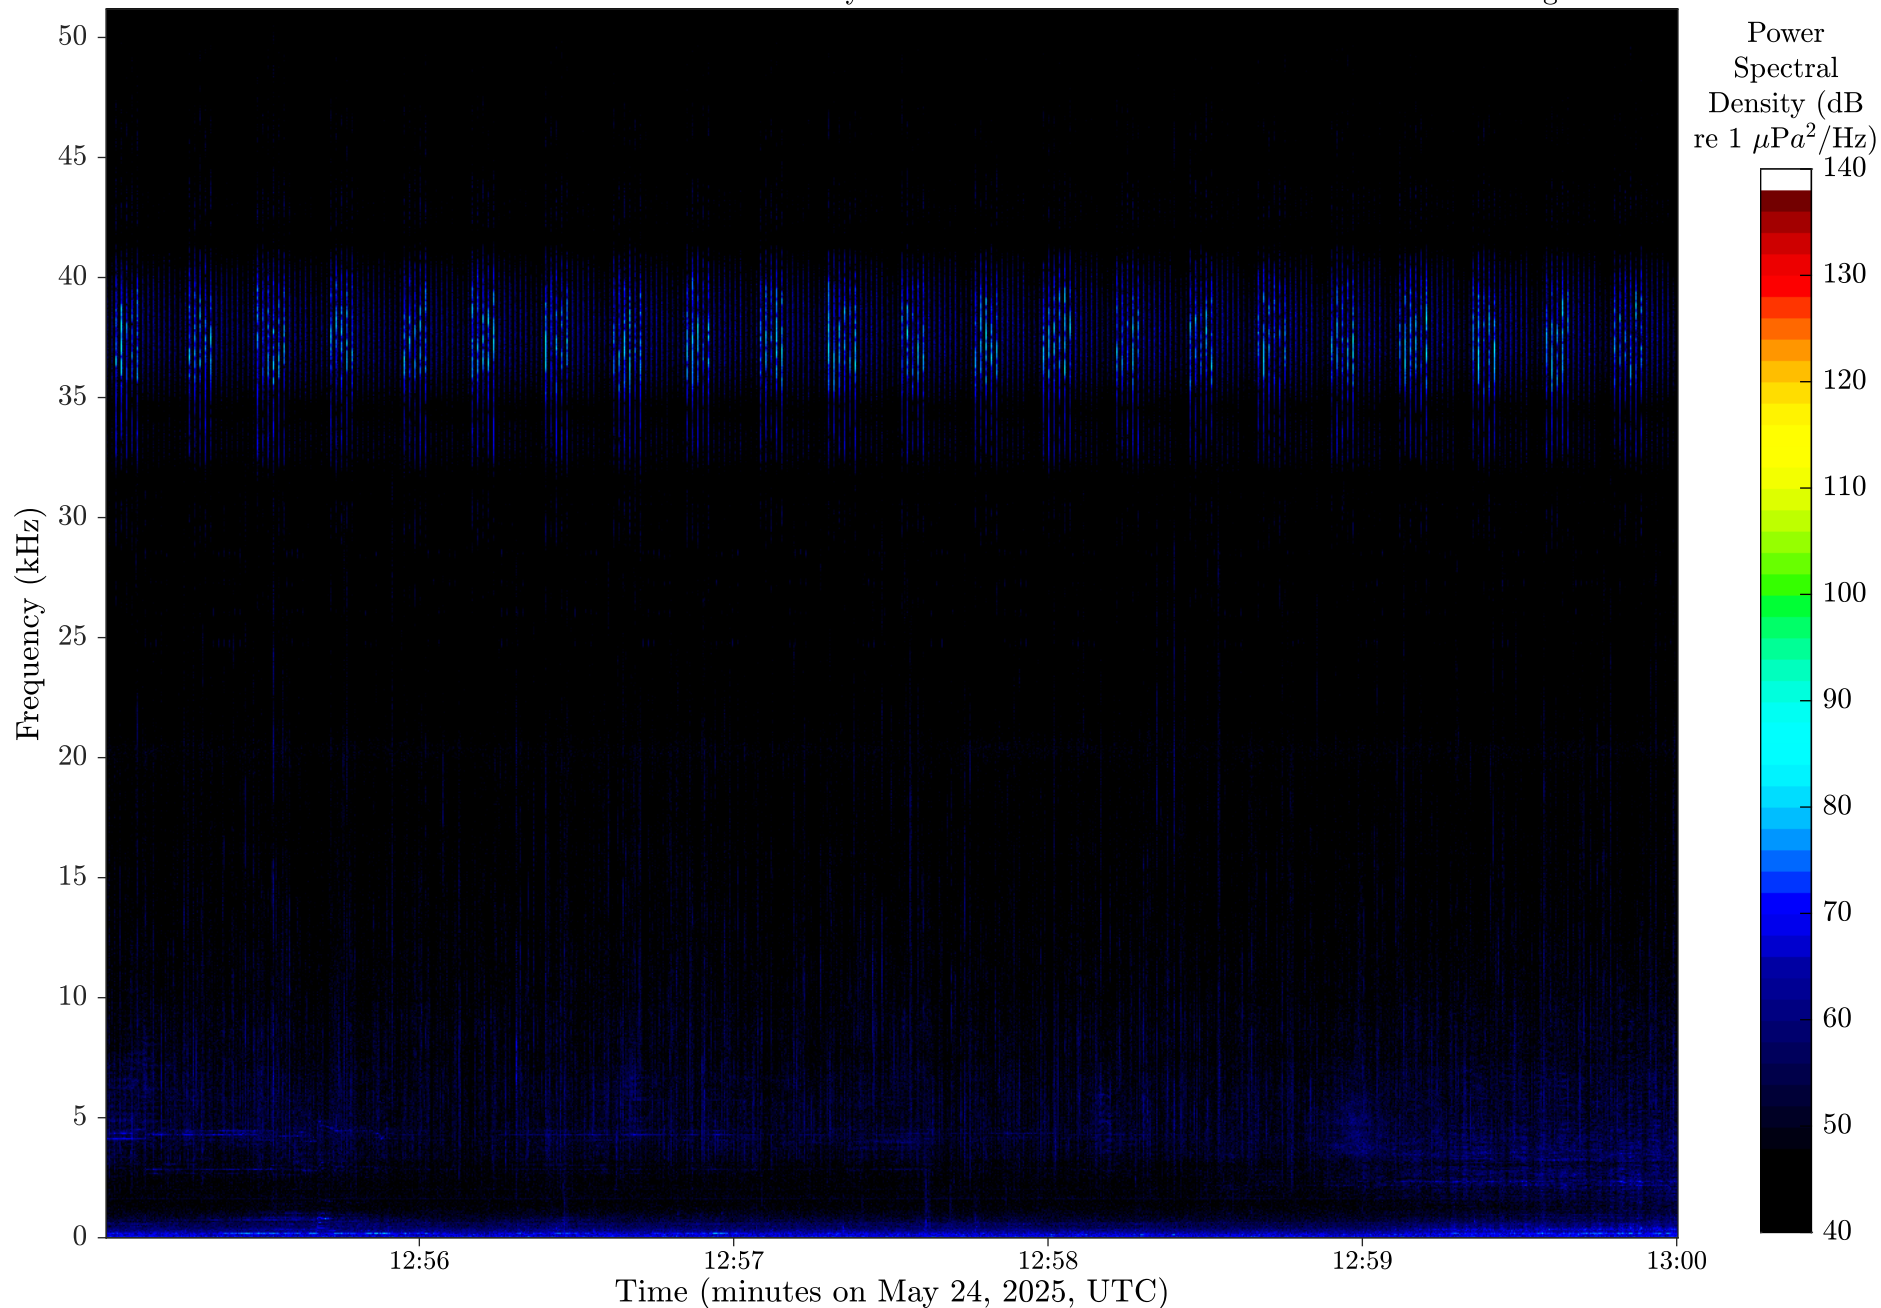


Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:36:38 UTC

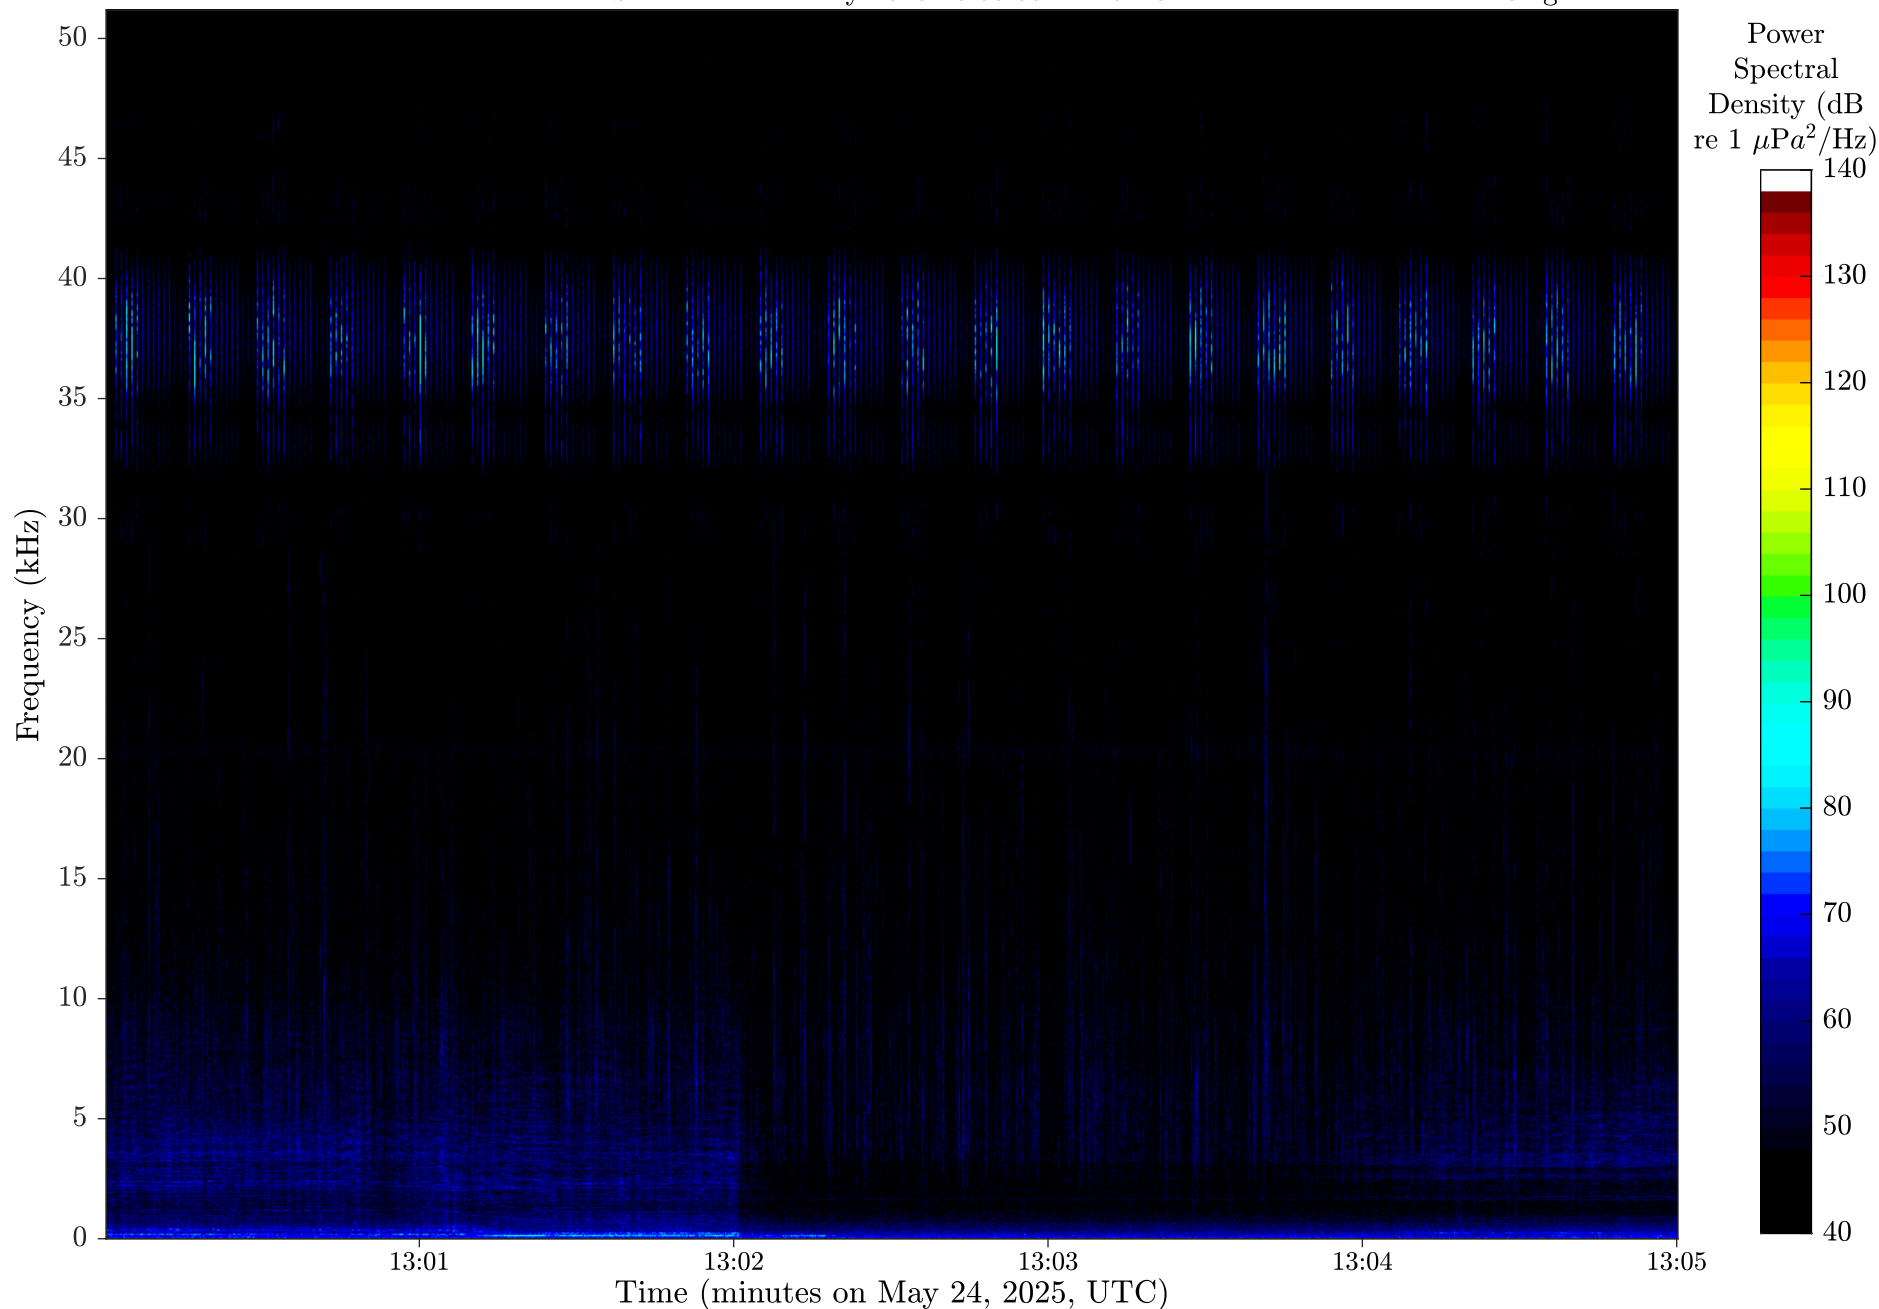


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:46 UTC

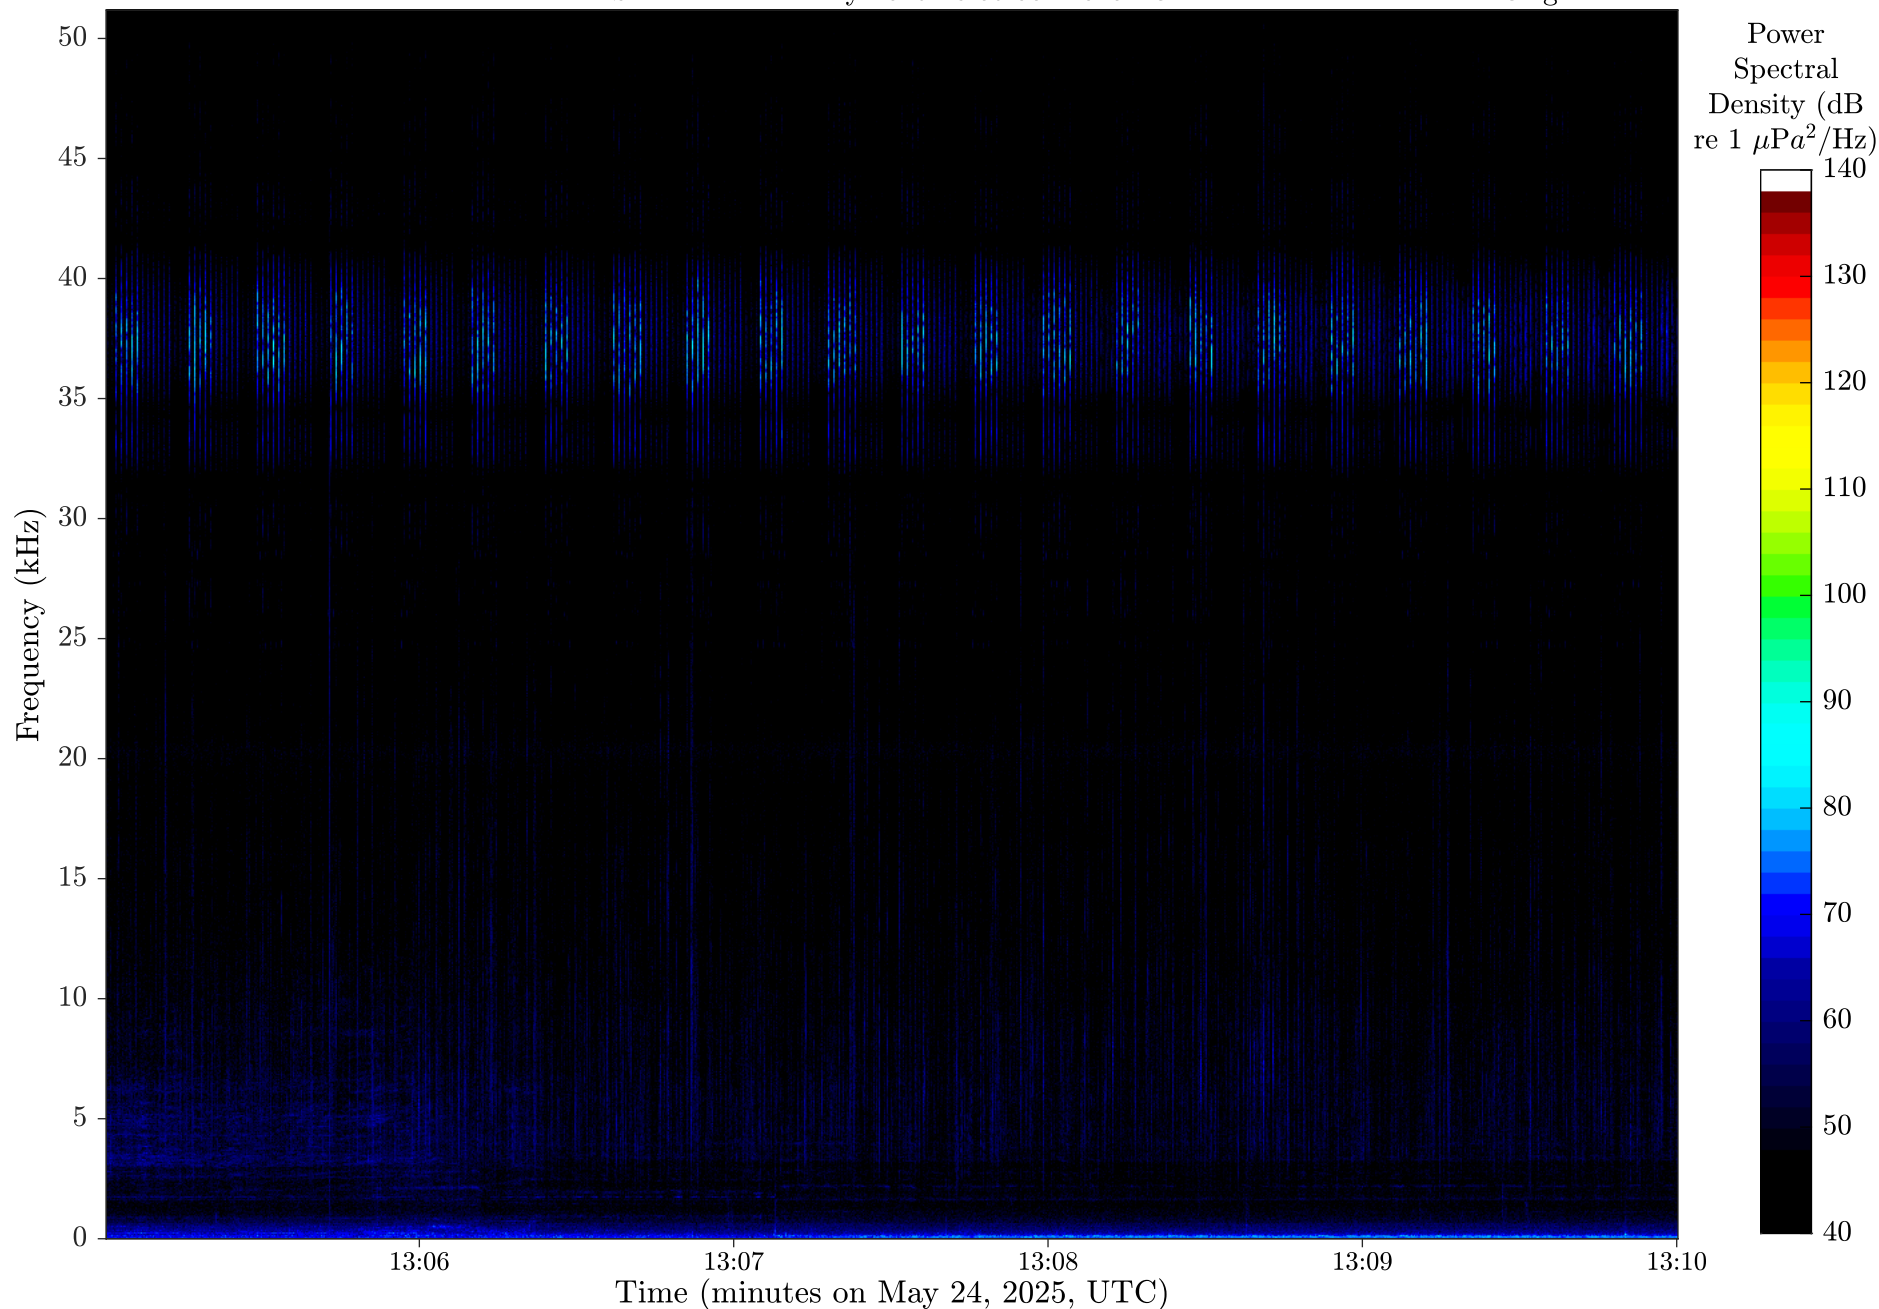


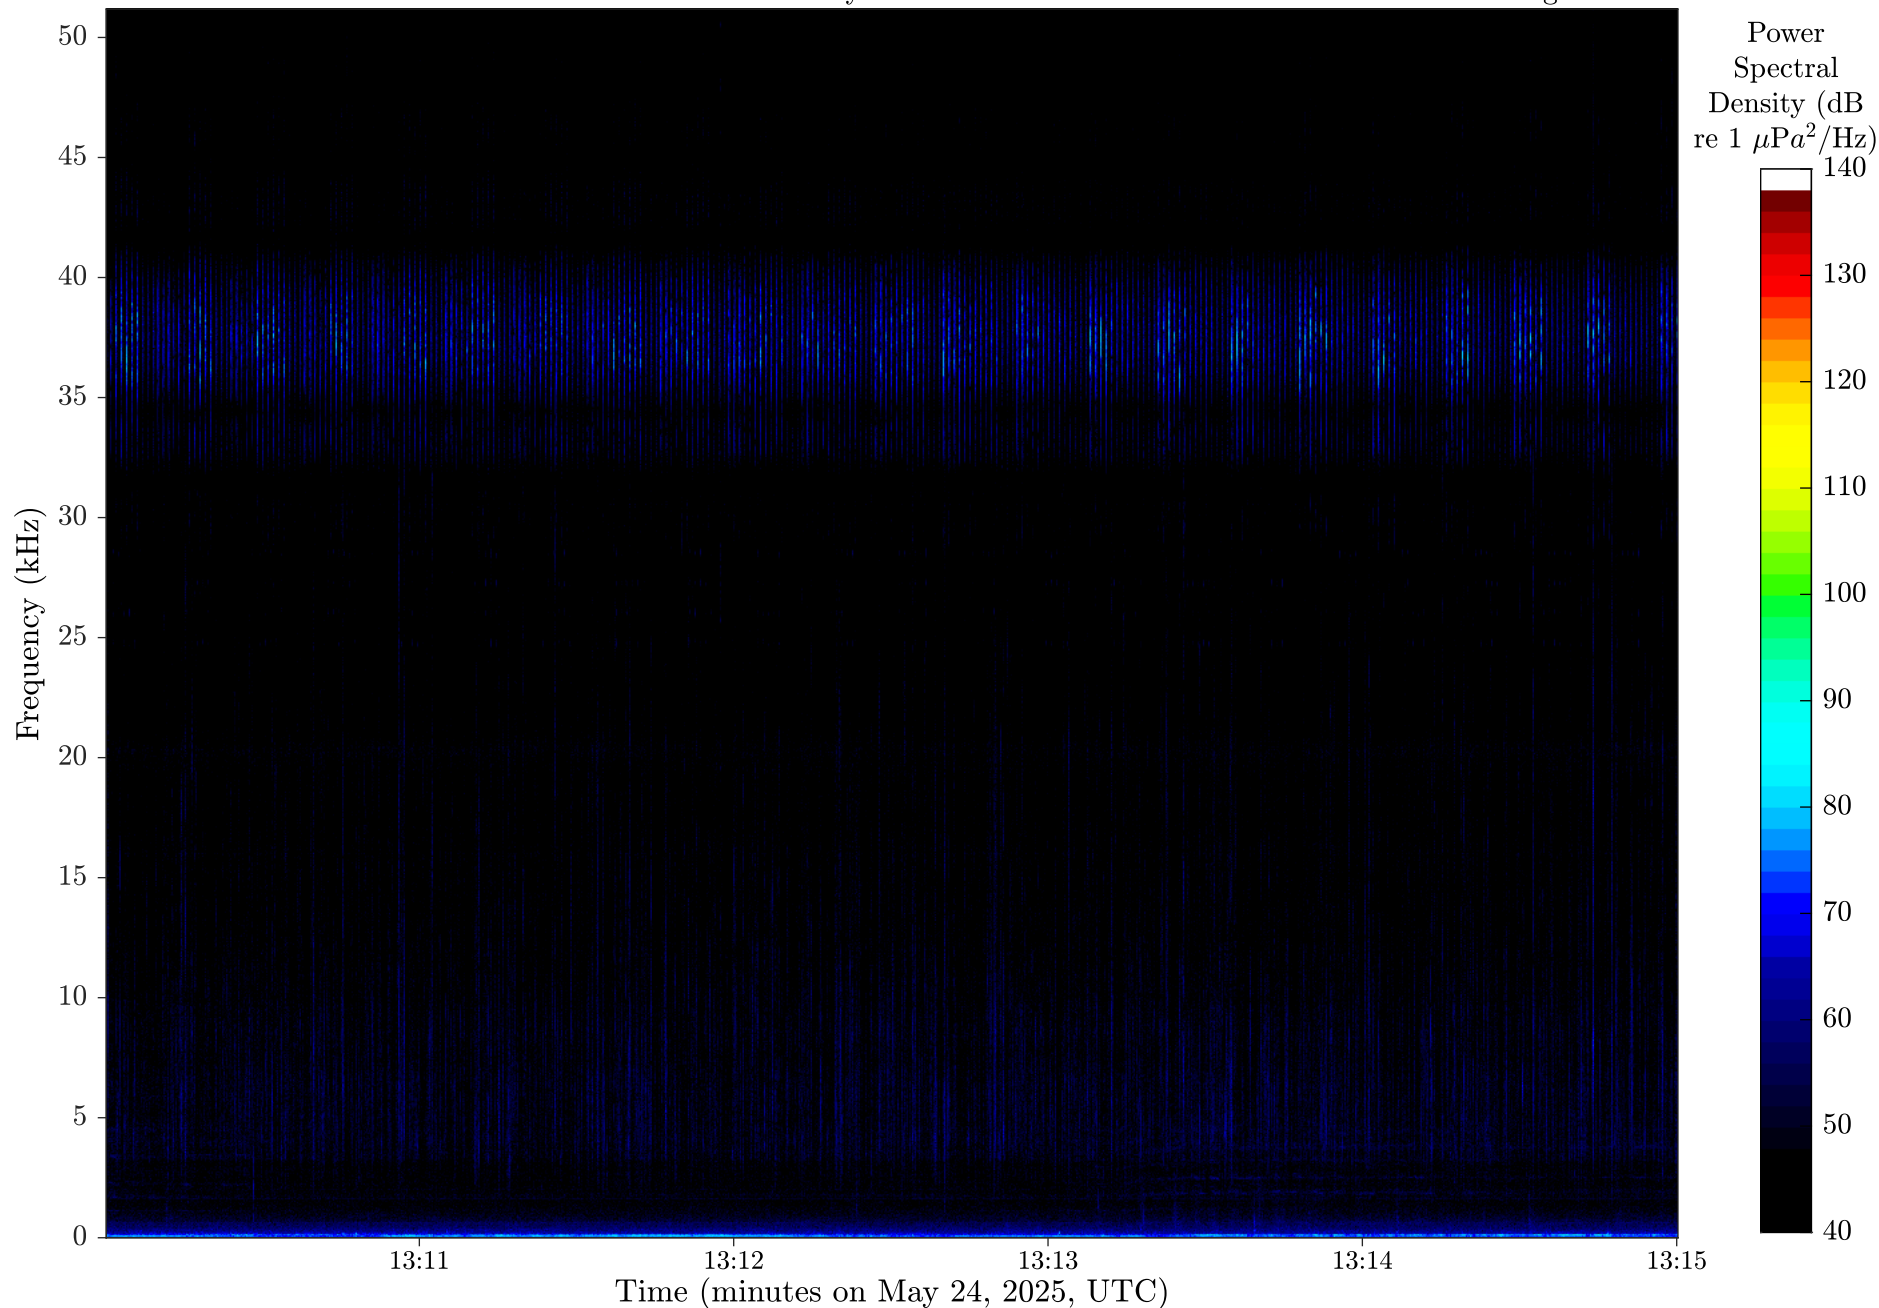

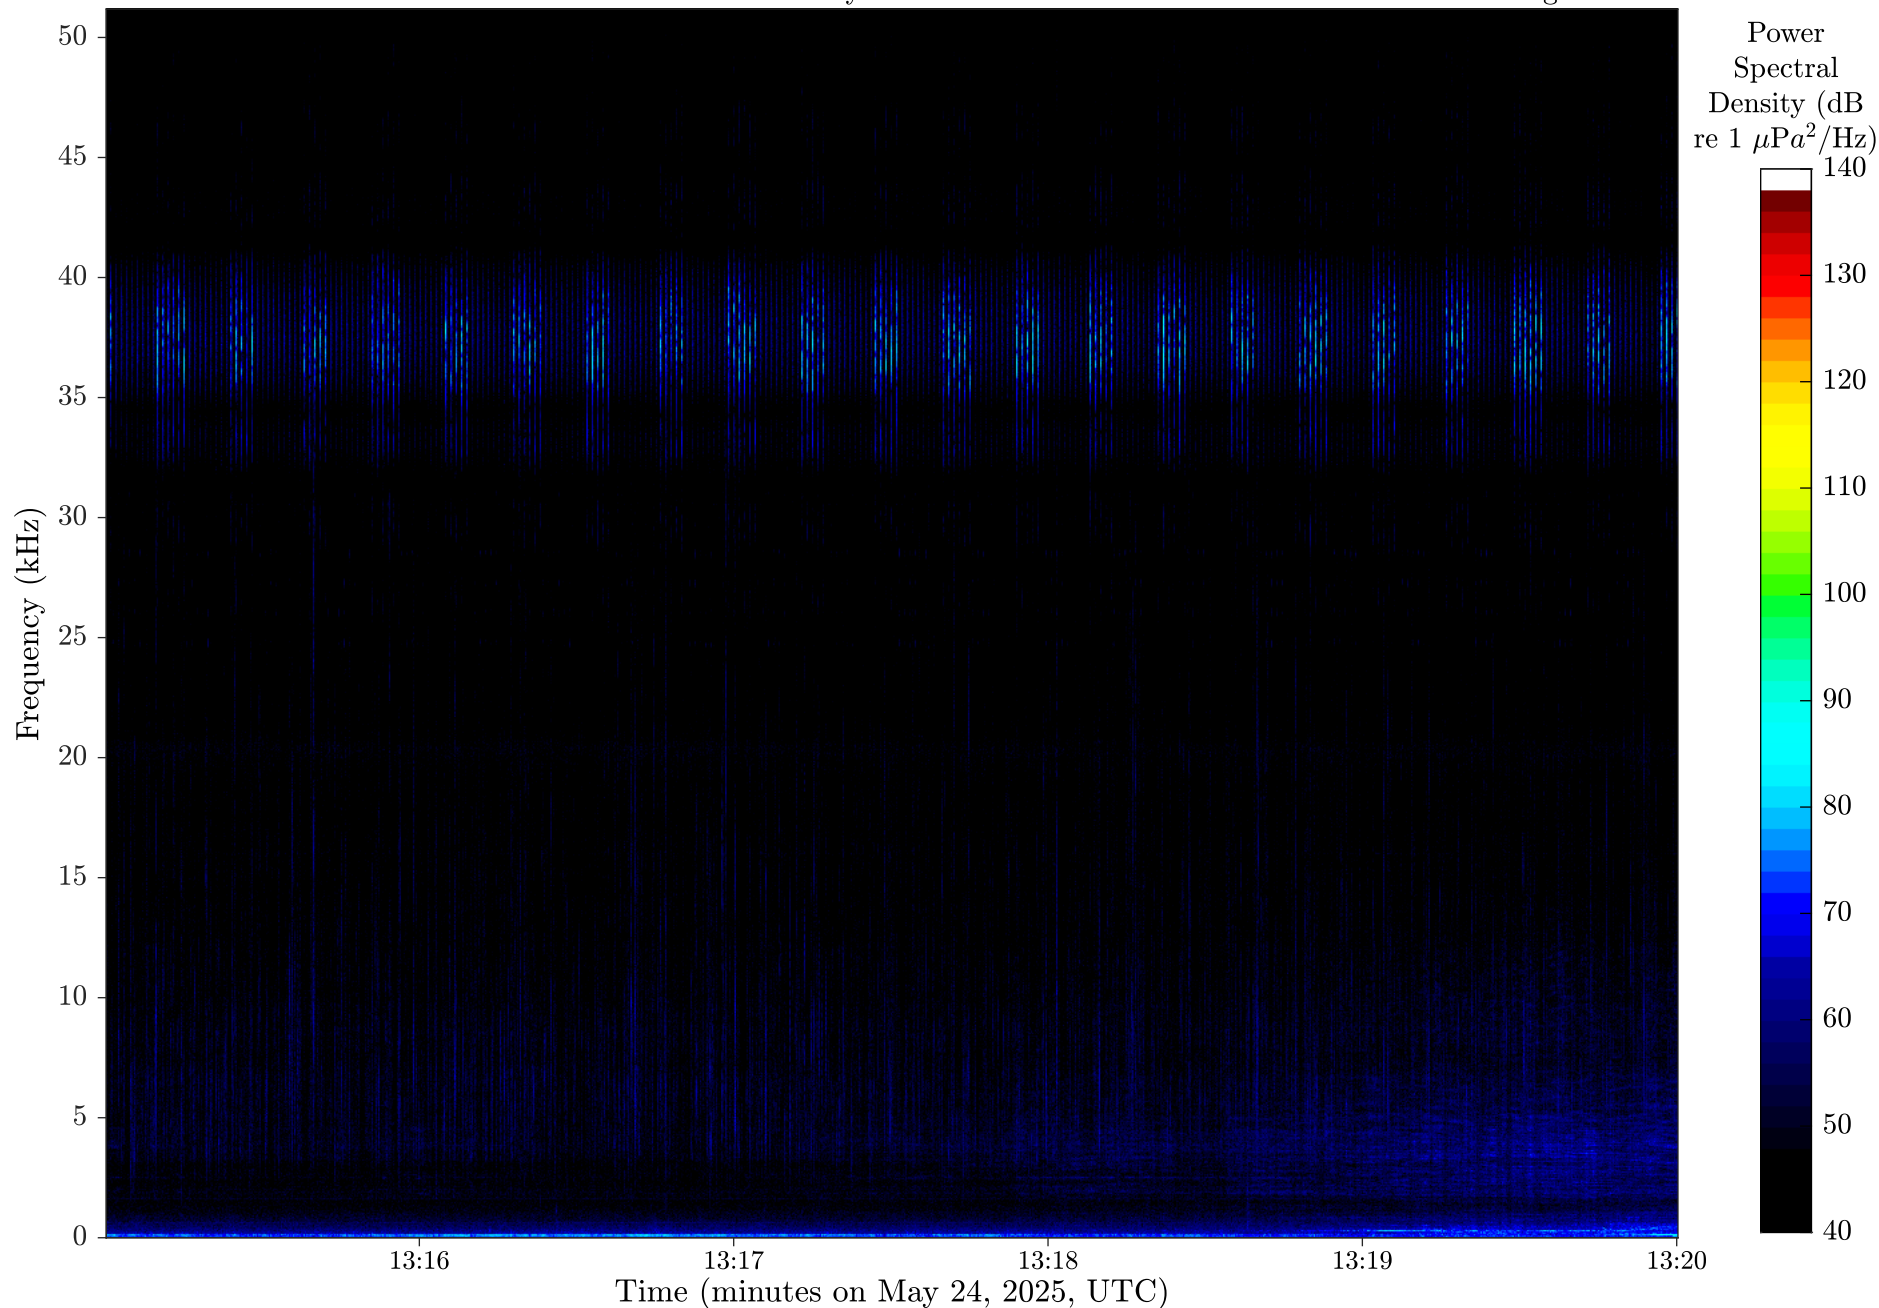


Comments: 30.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:10 UTC

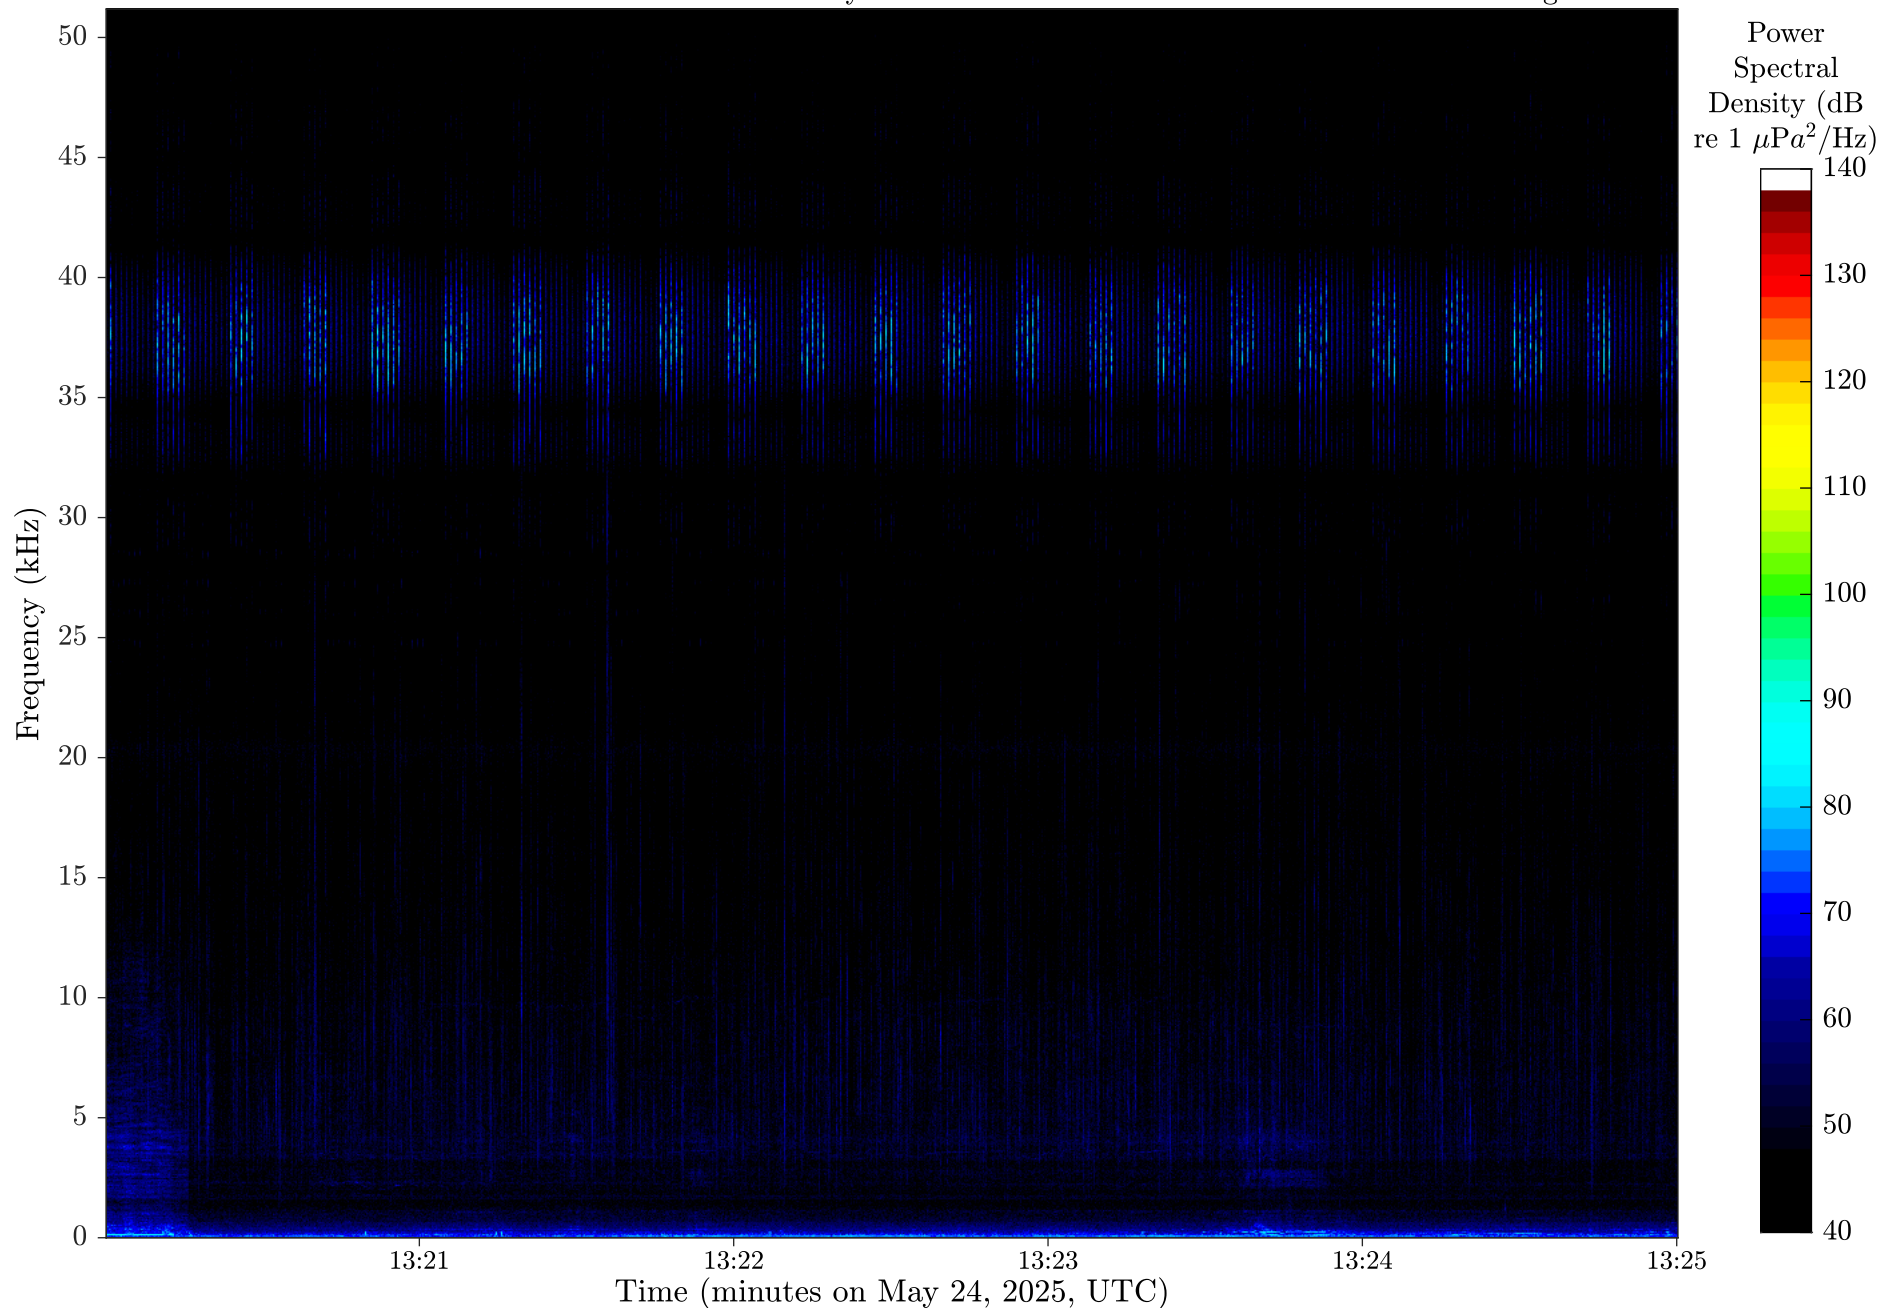


Comments: 31.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:18 UTC

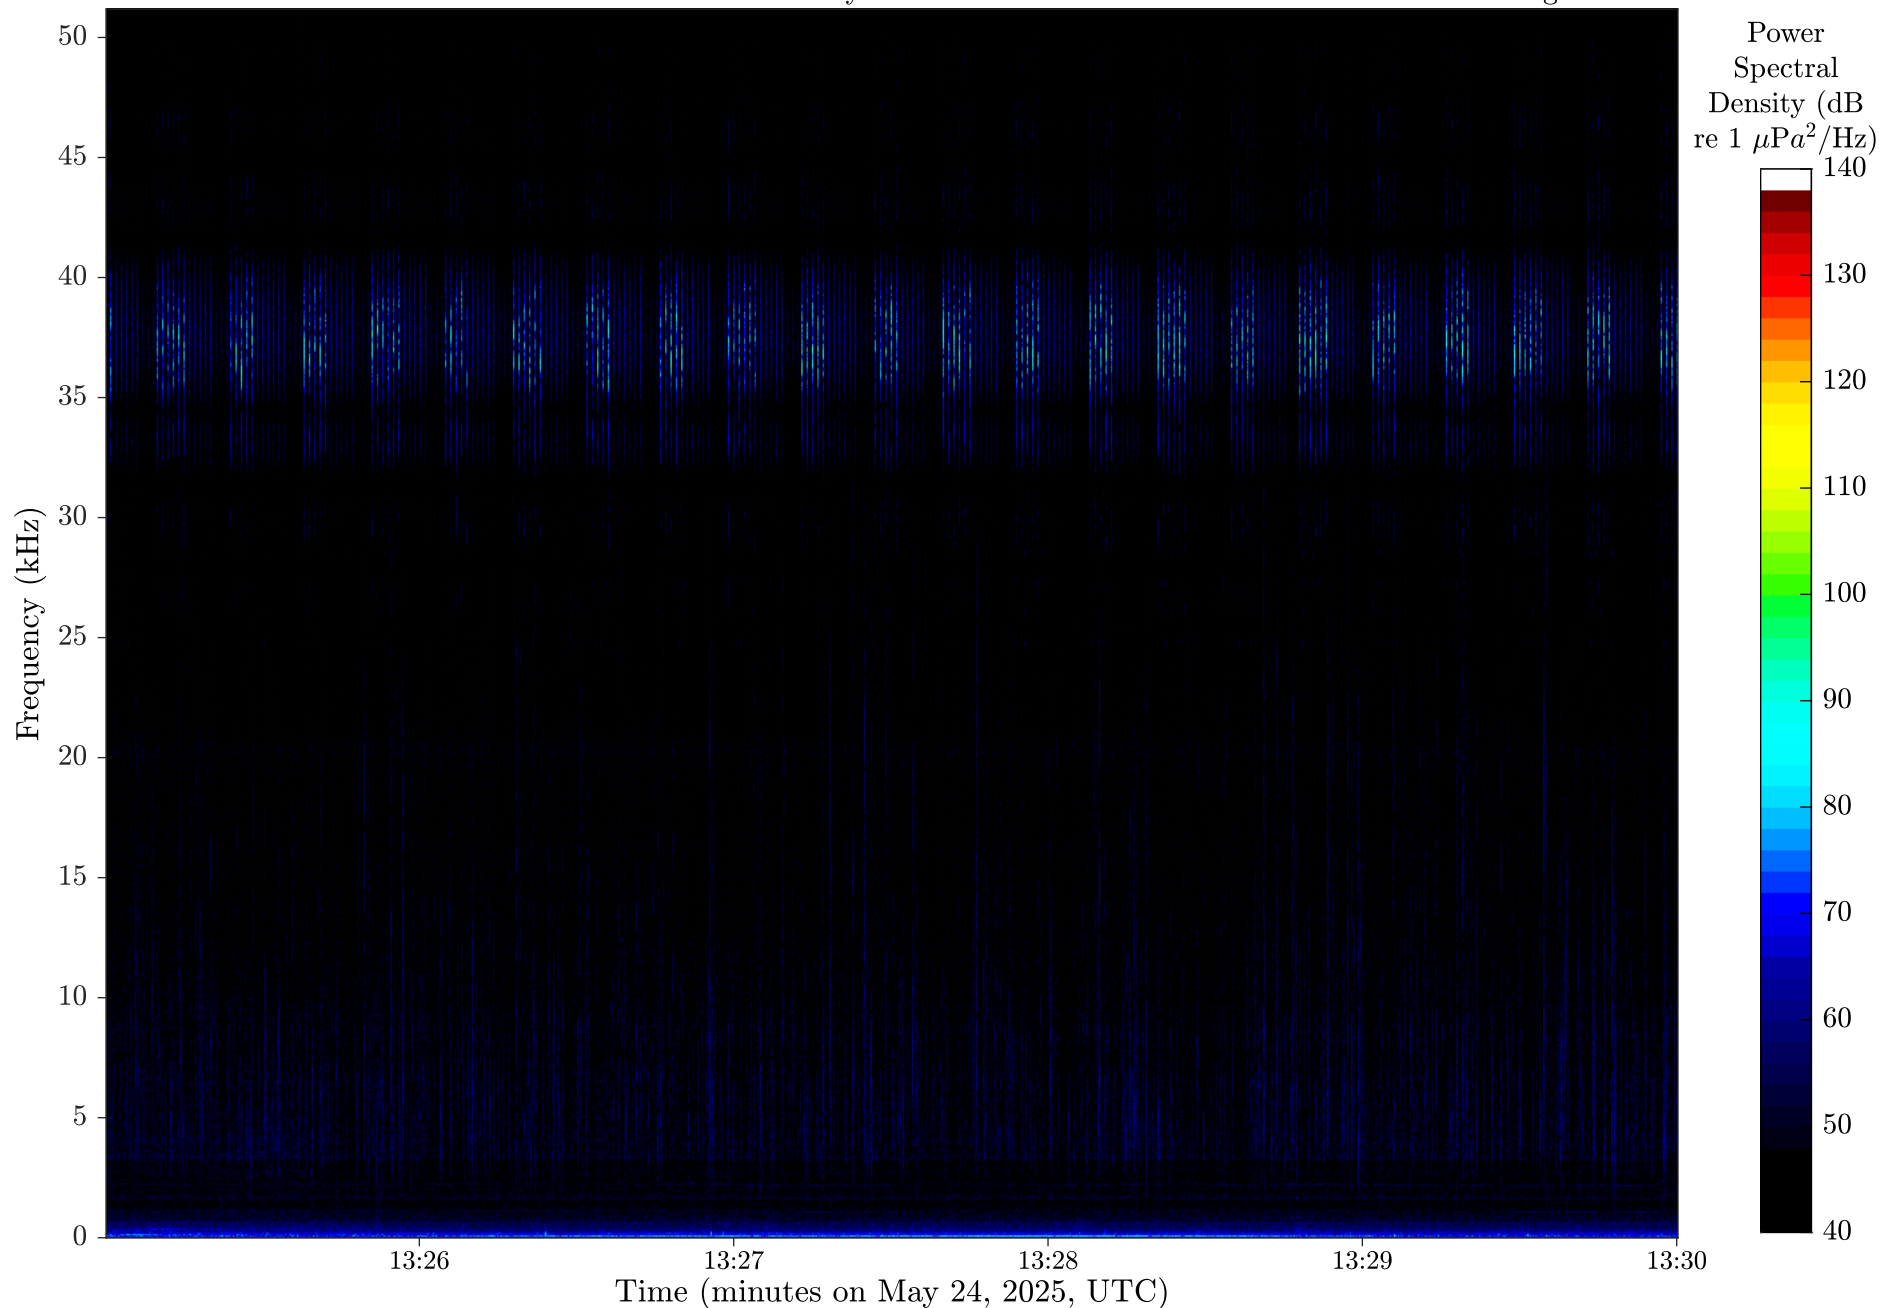


Comments: 32.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:25 UTC

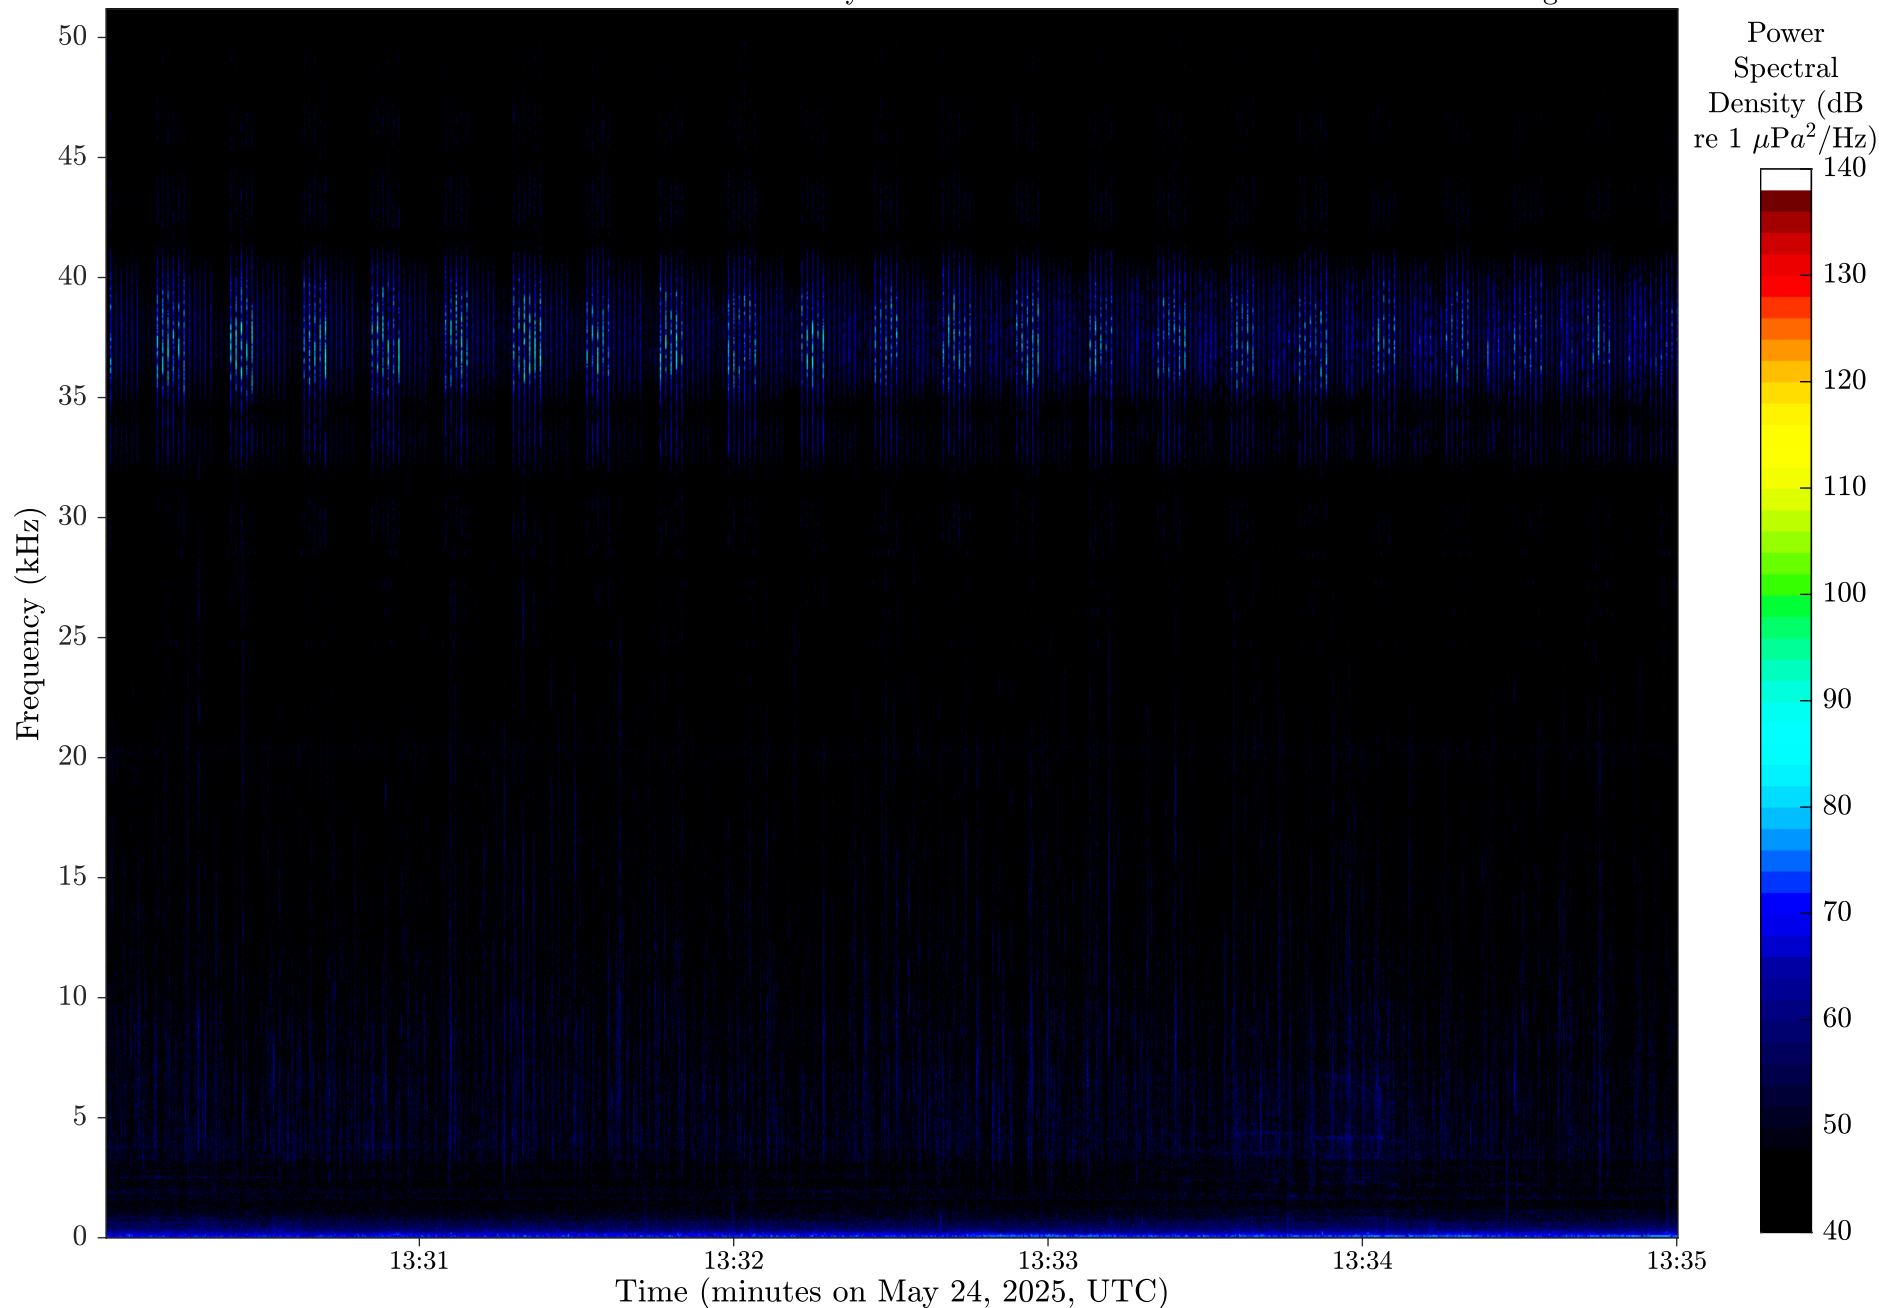


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:34 UTC

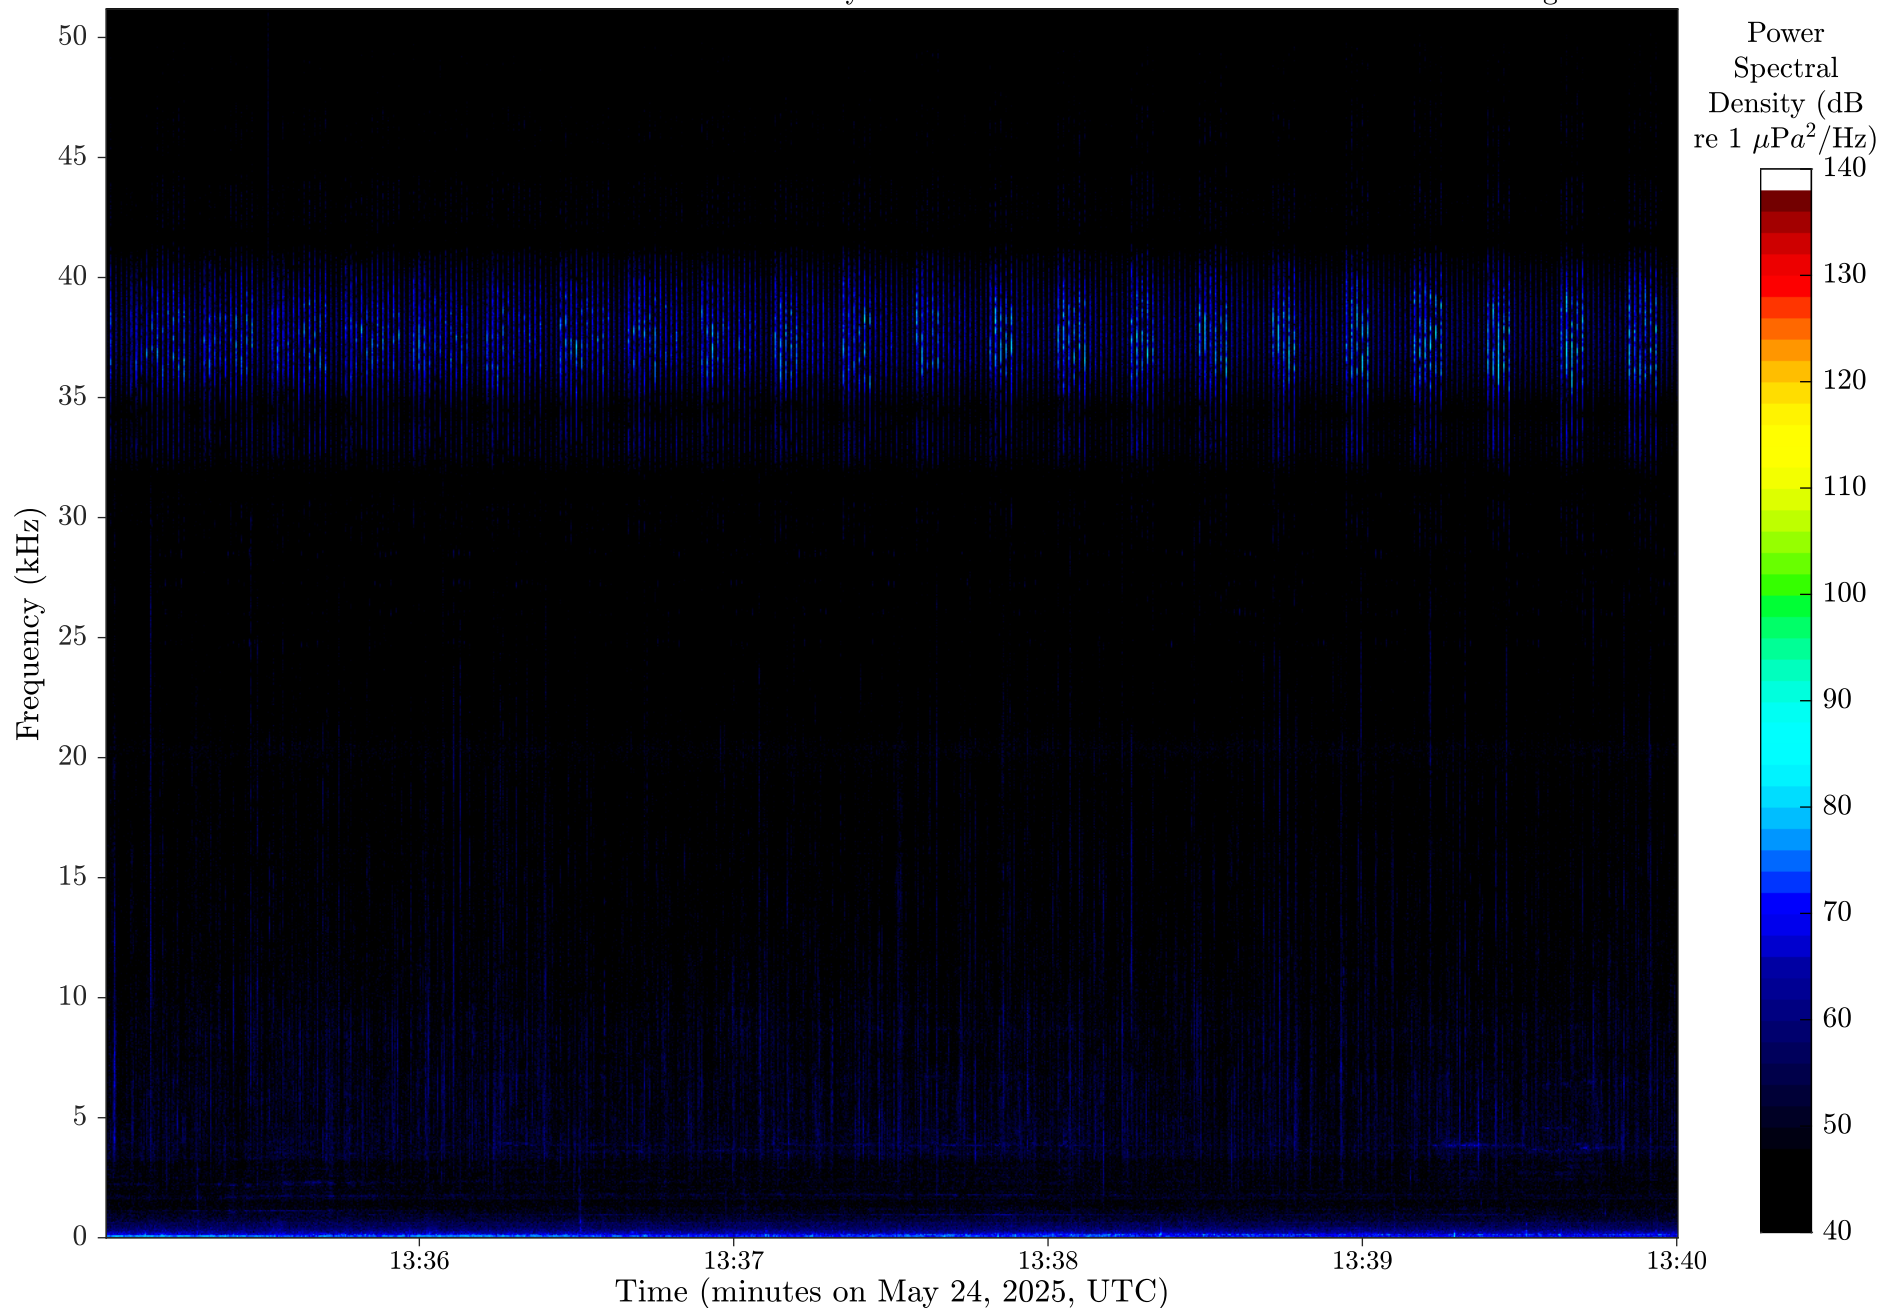


Comments: 30.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:42 UTC

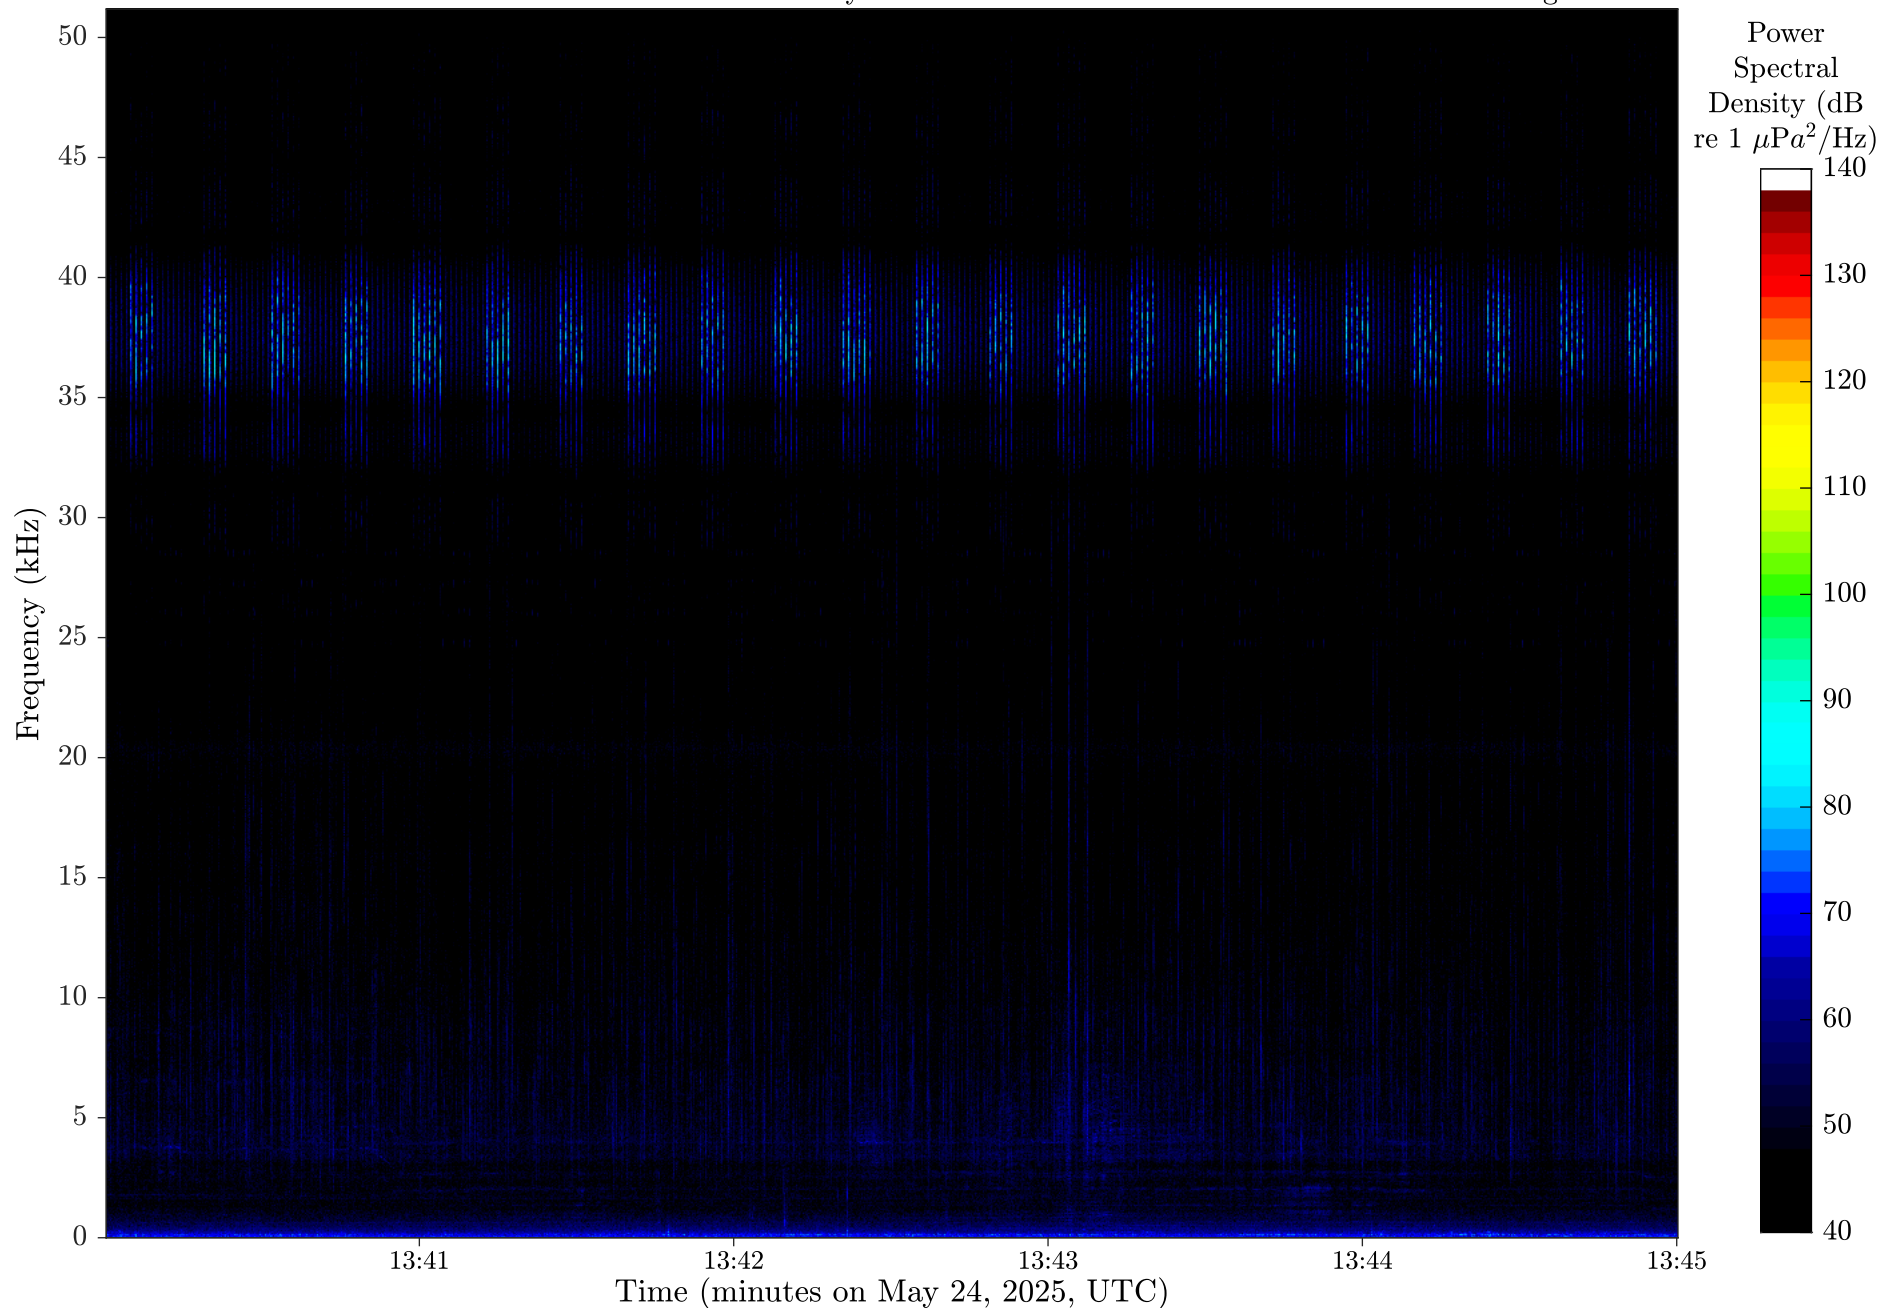


Comments: 31.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:50 UTC

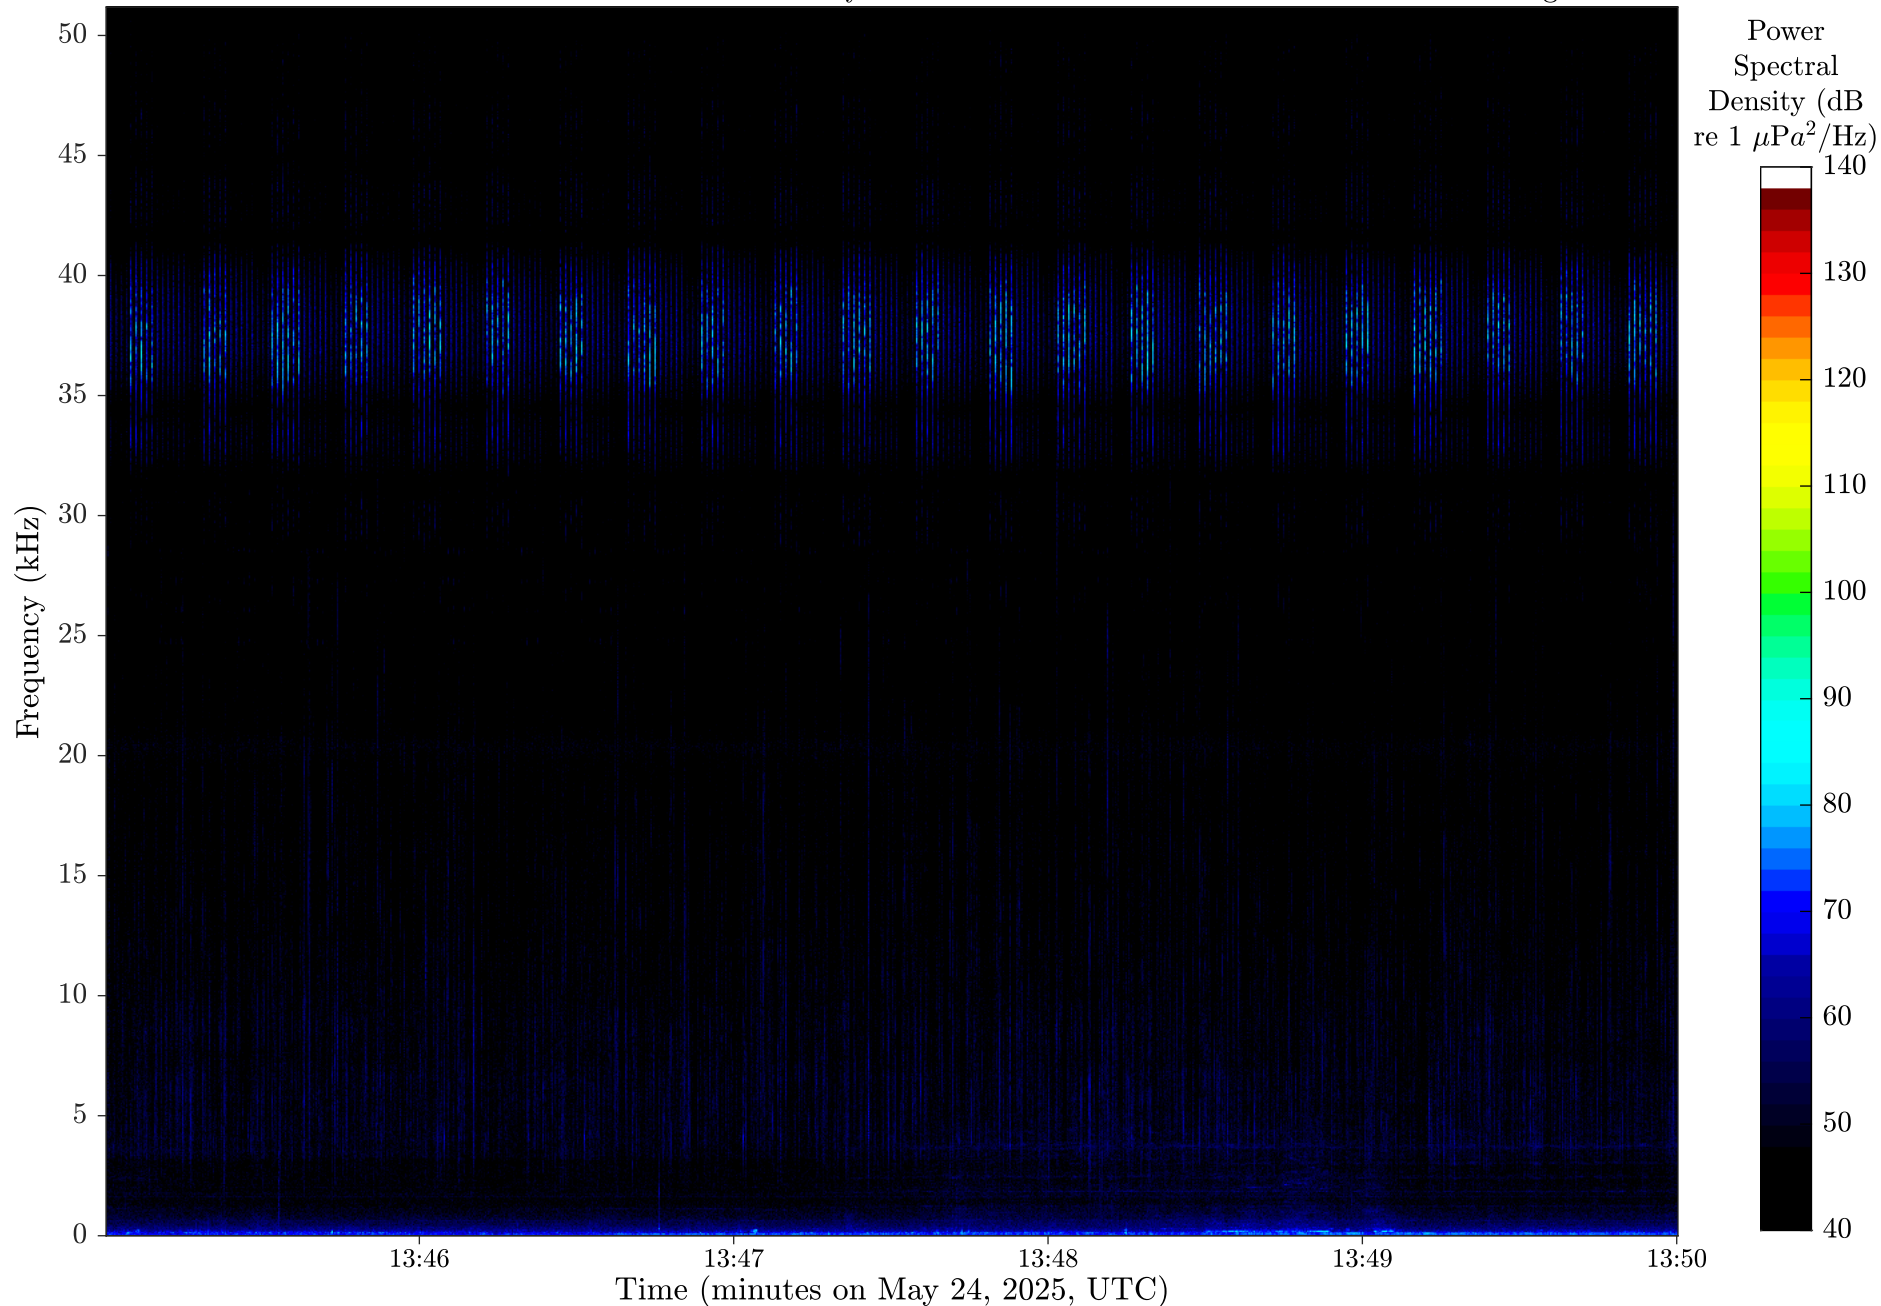


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:58 UTC

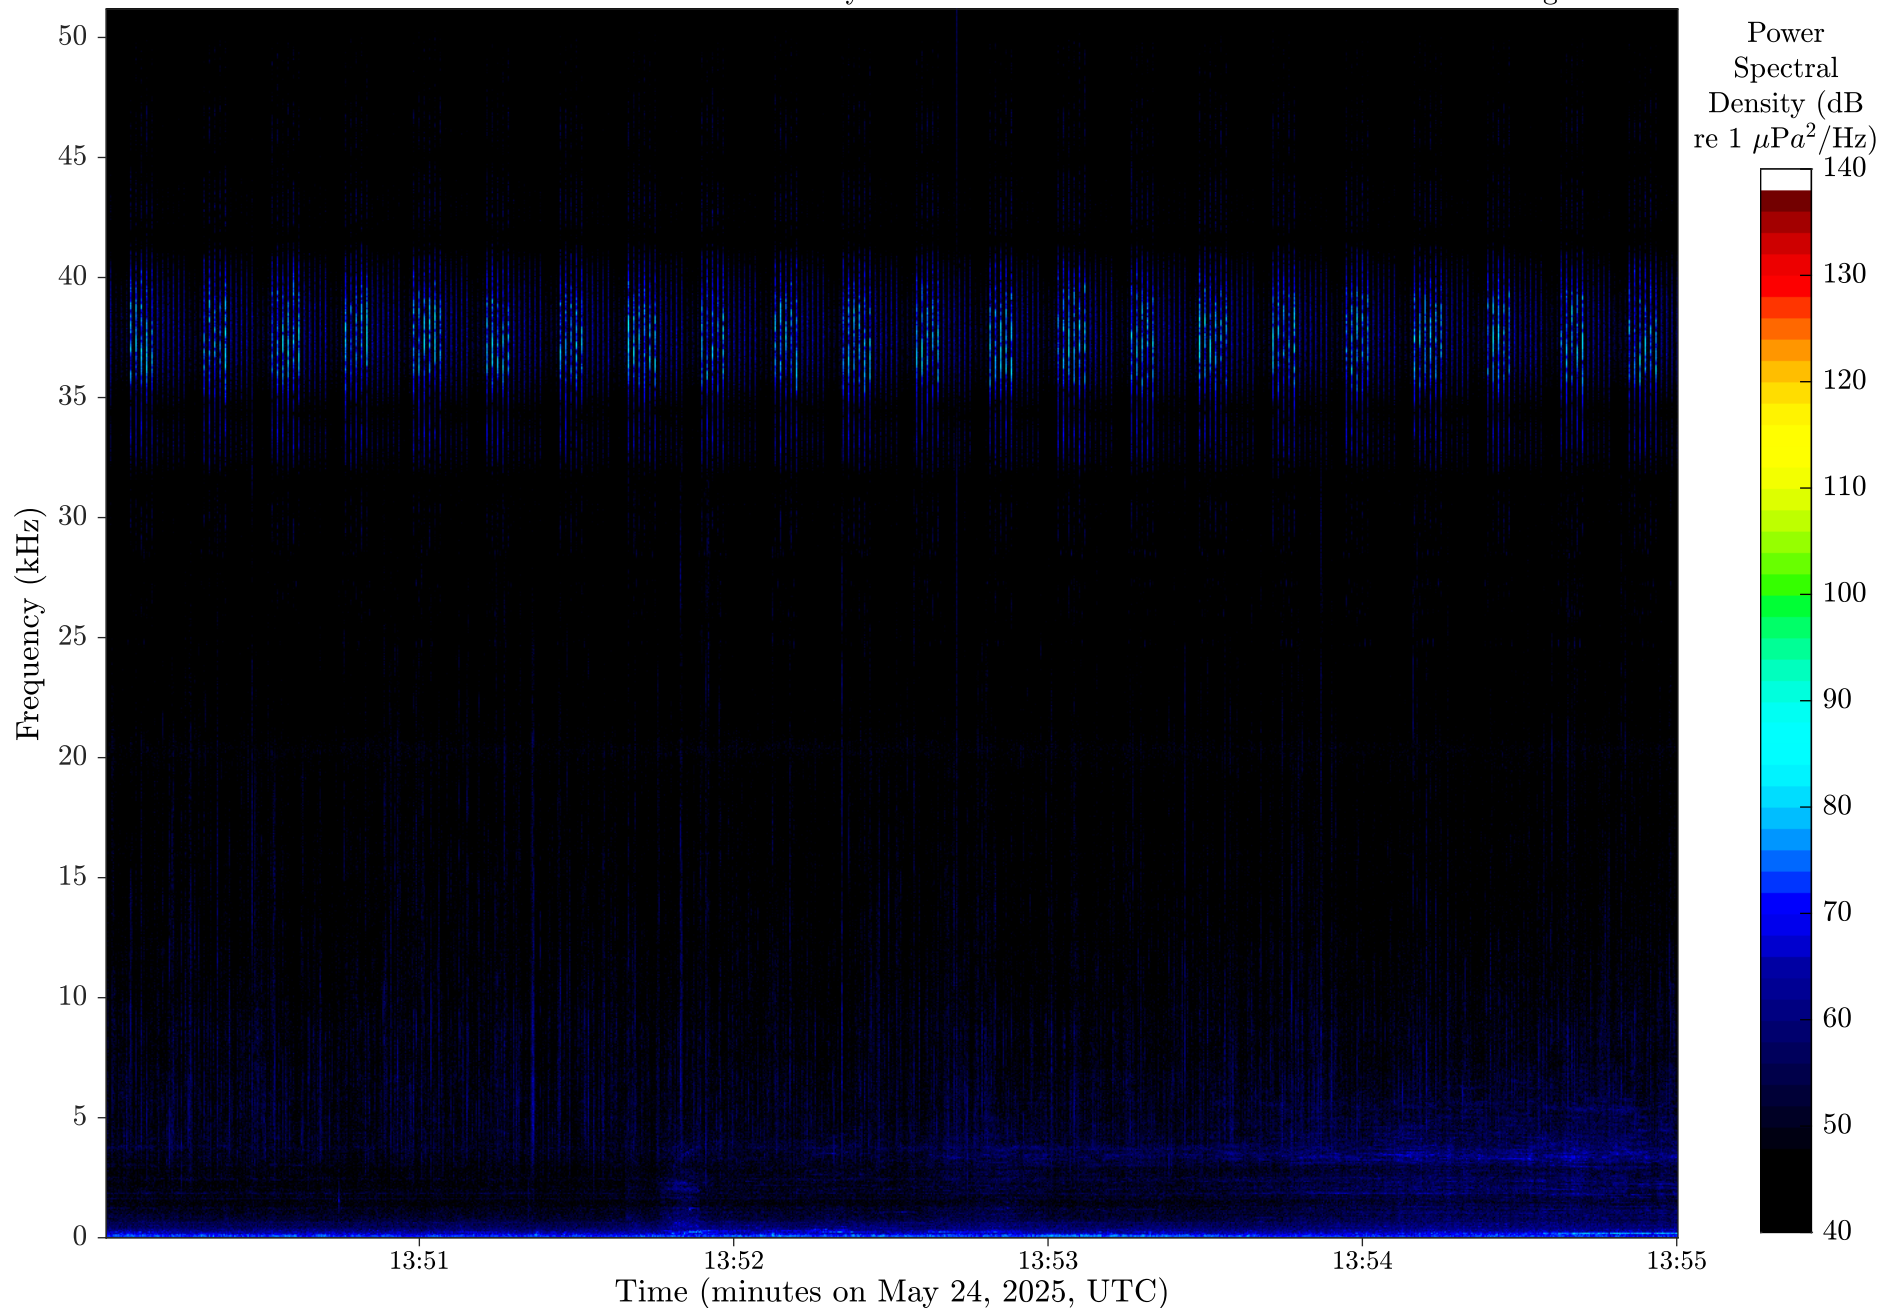


Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:06 UTC

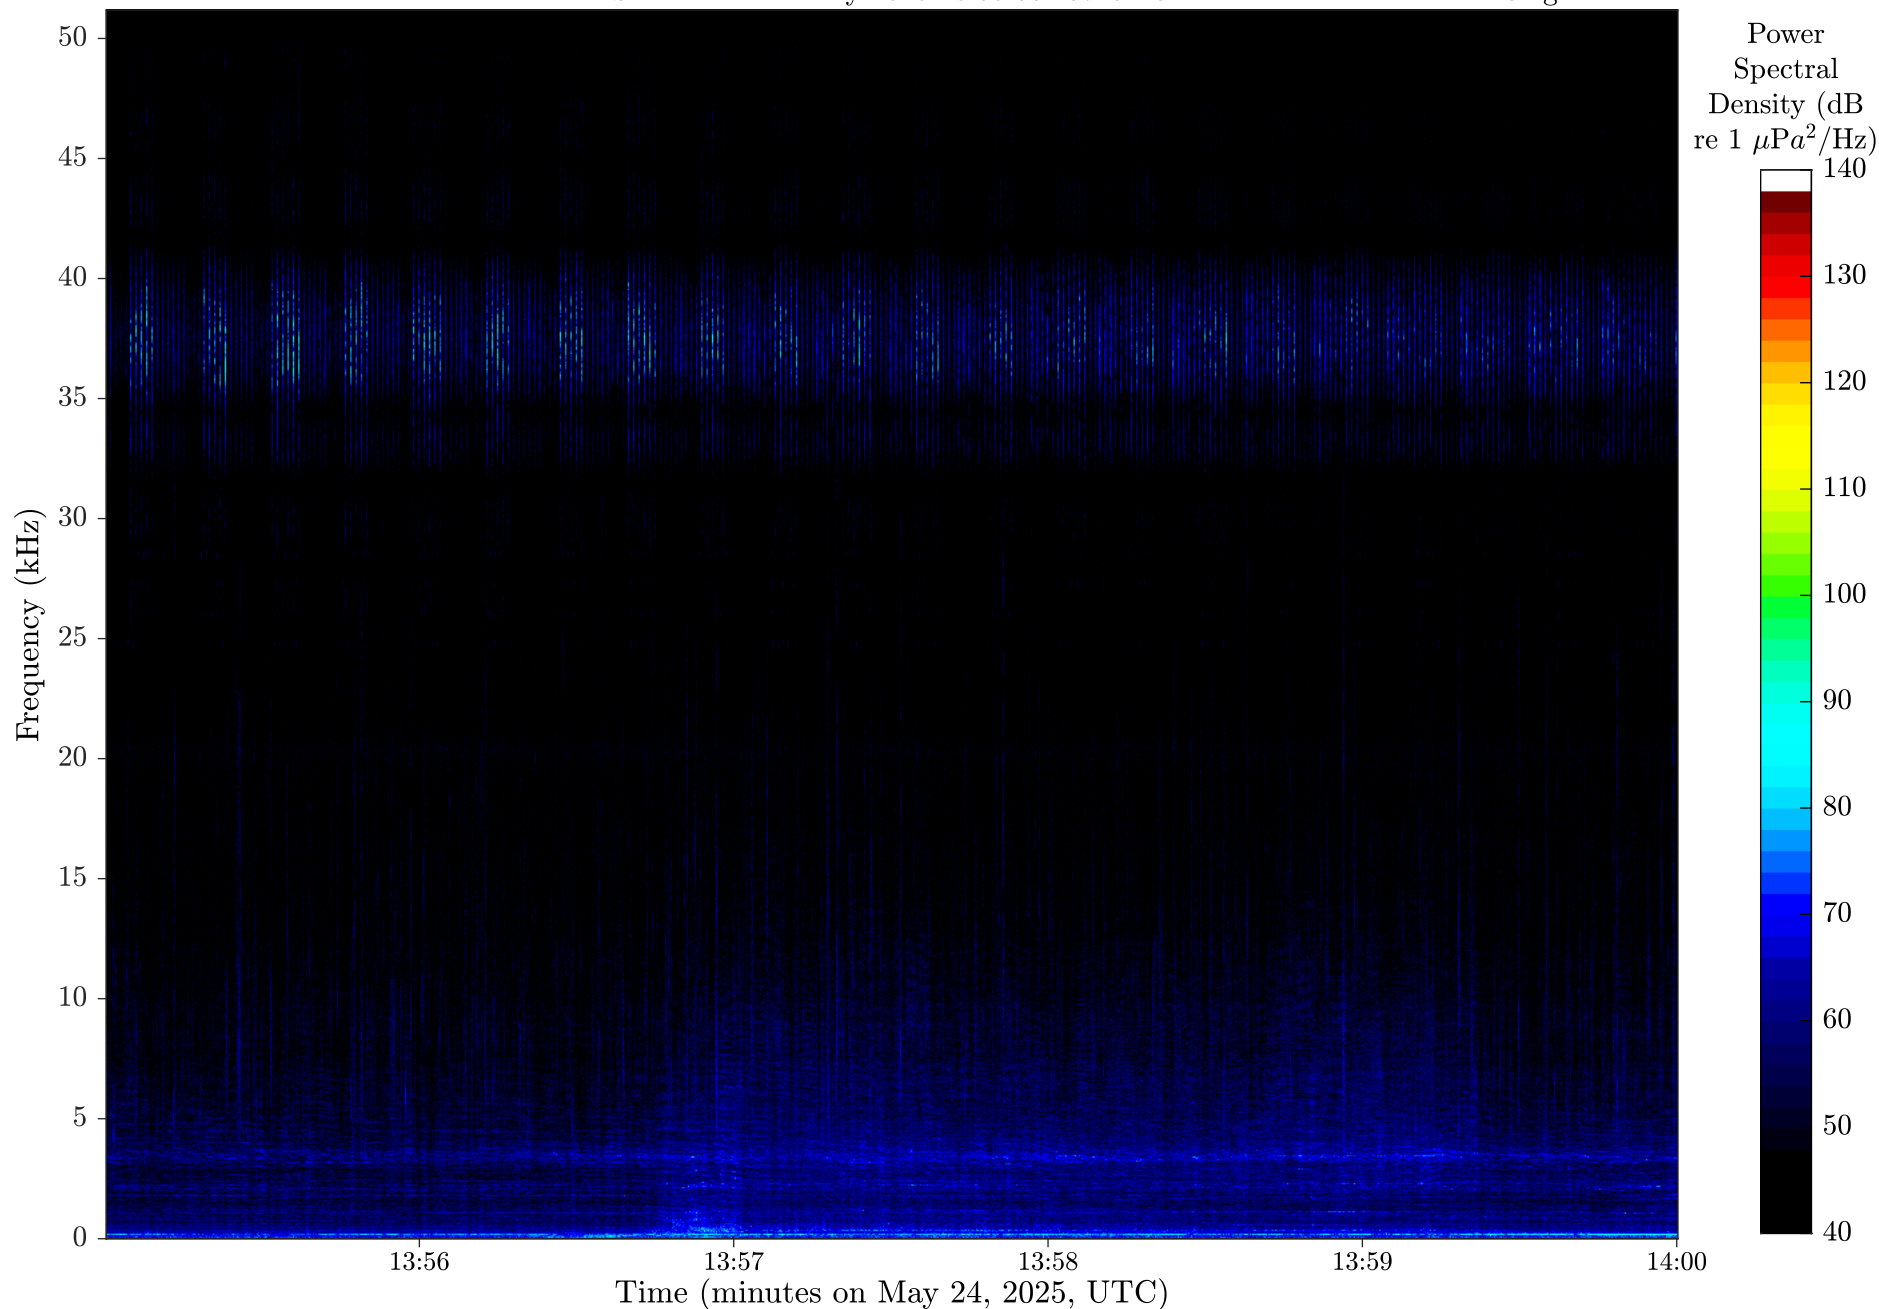


Comments: 29.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:15 UTC

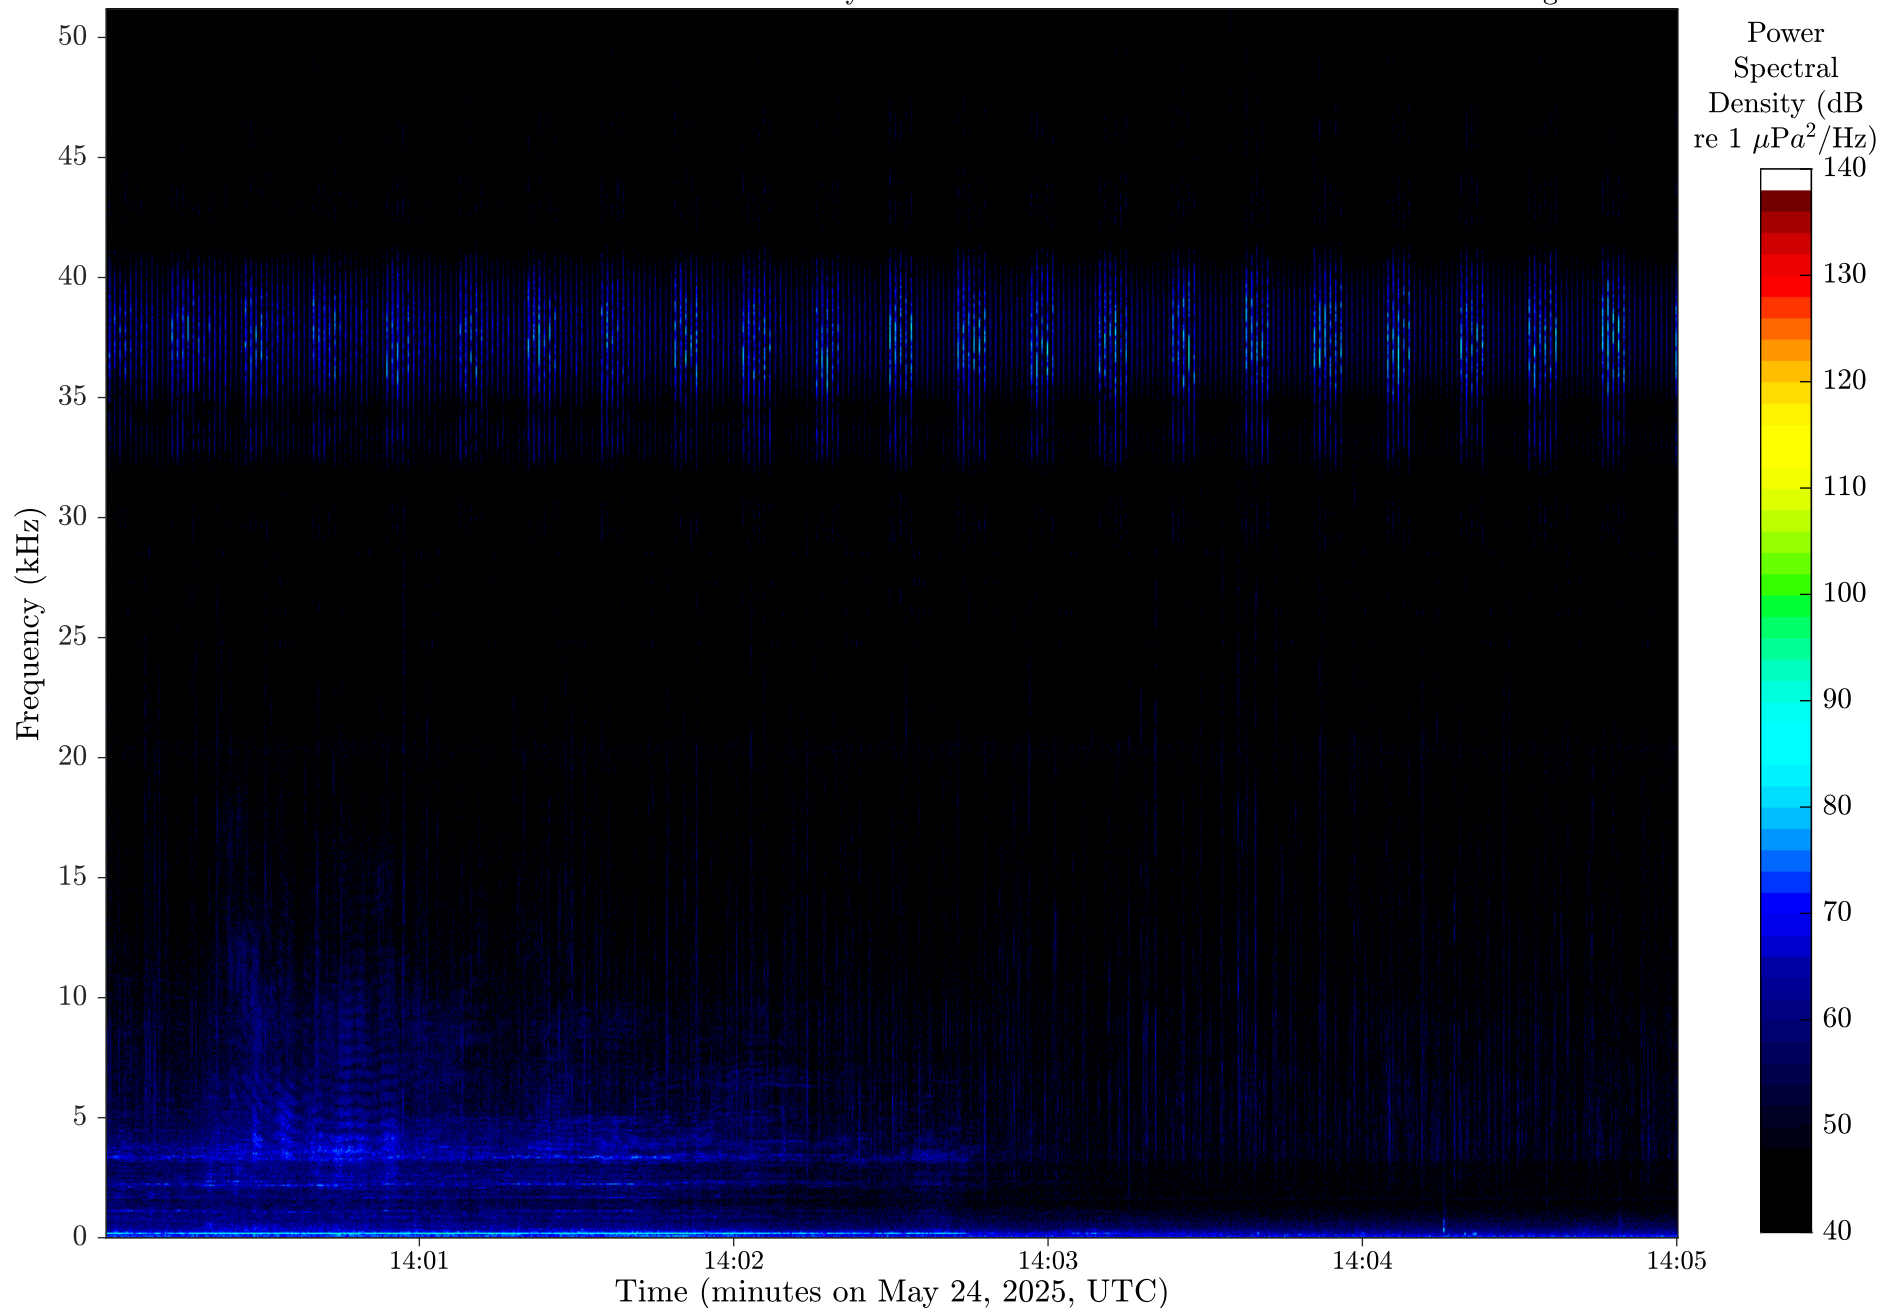


Comments: 31.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:23 UTC

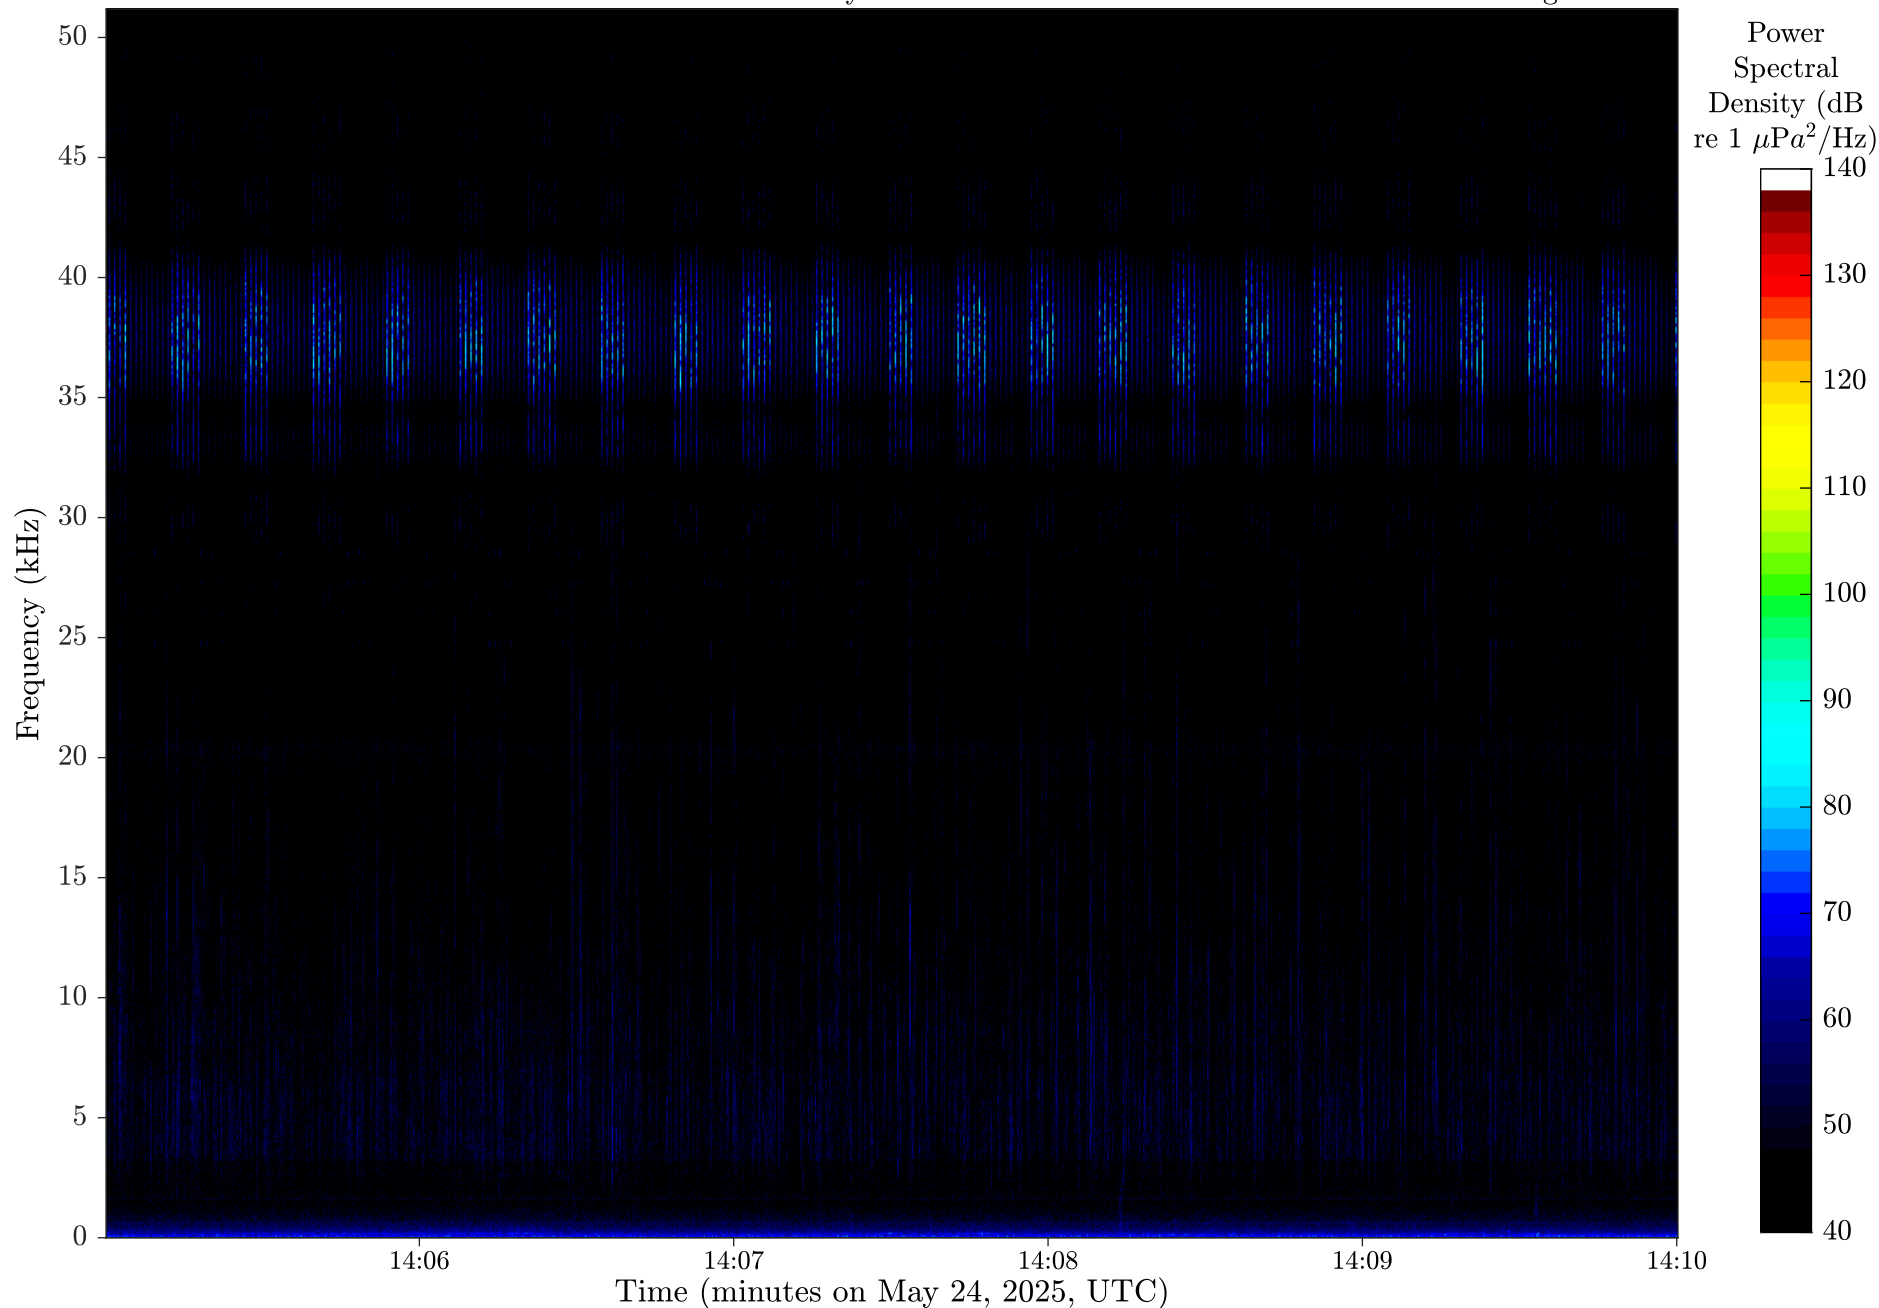


Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:32 UTC

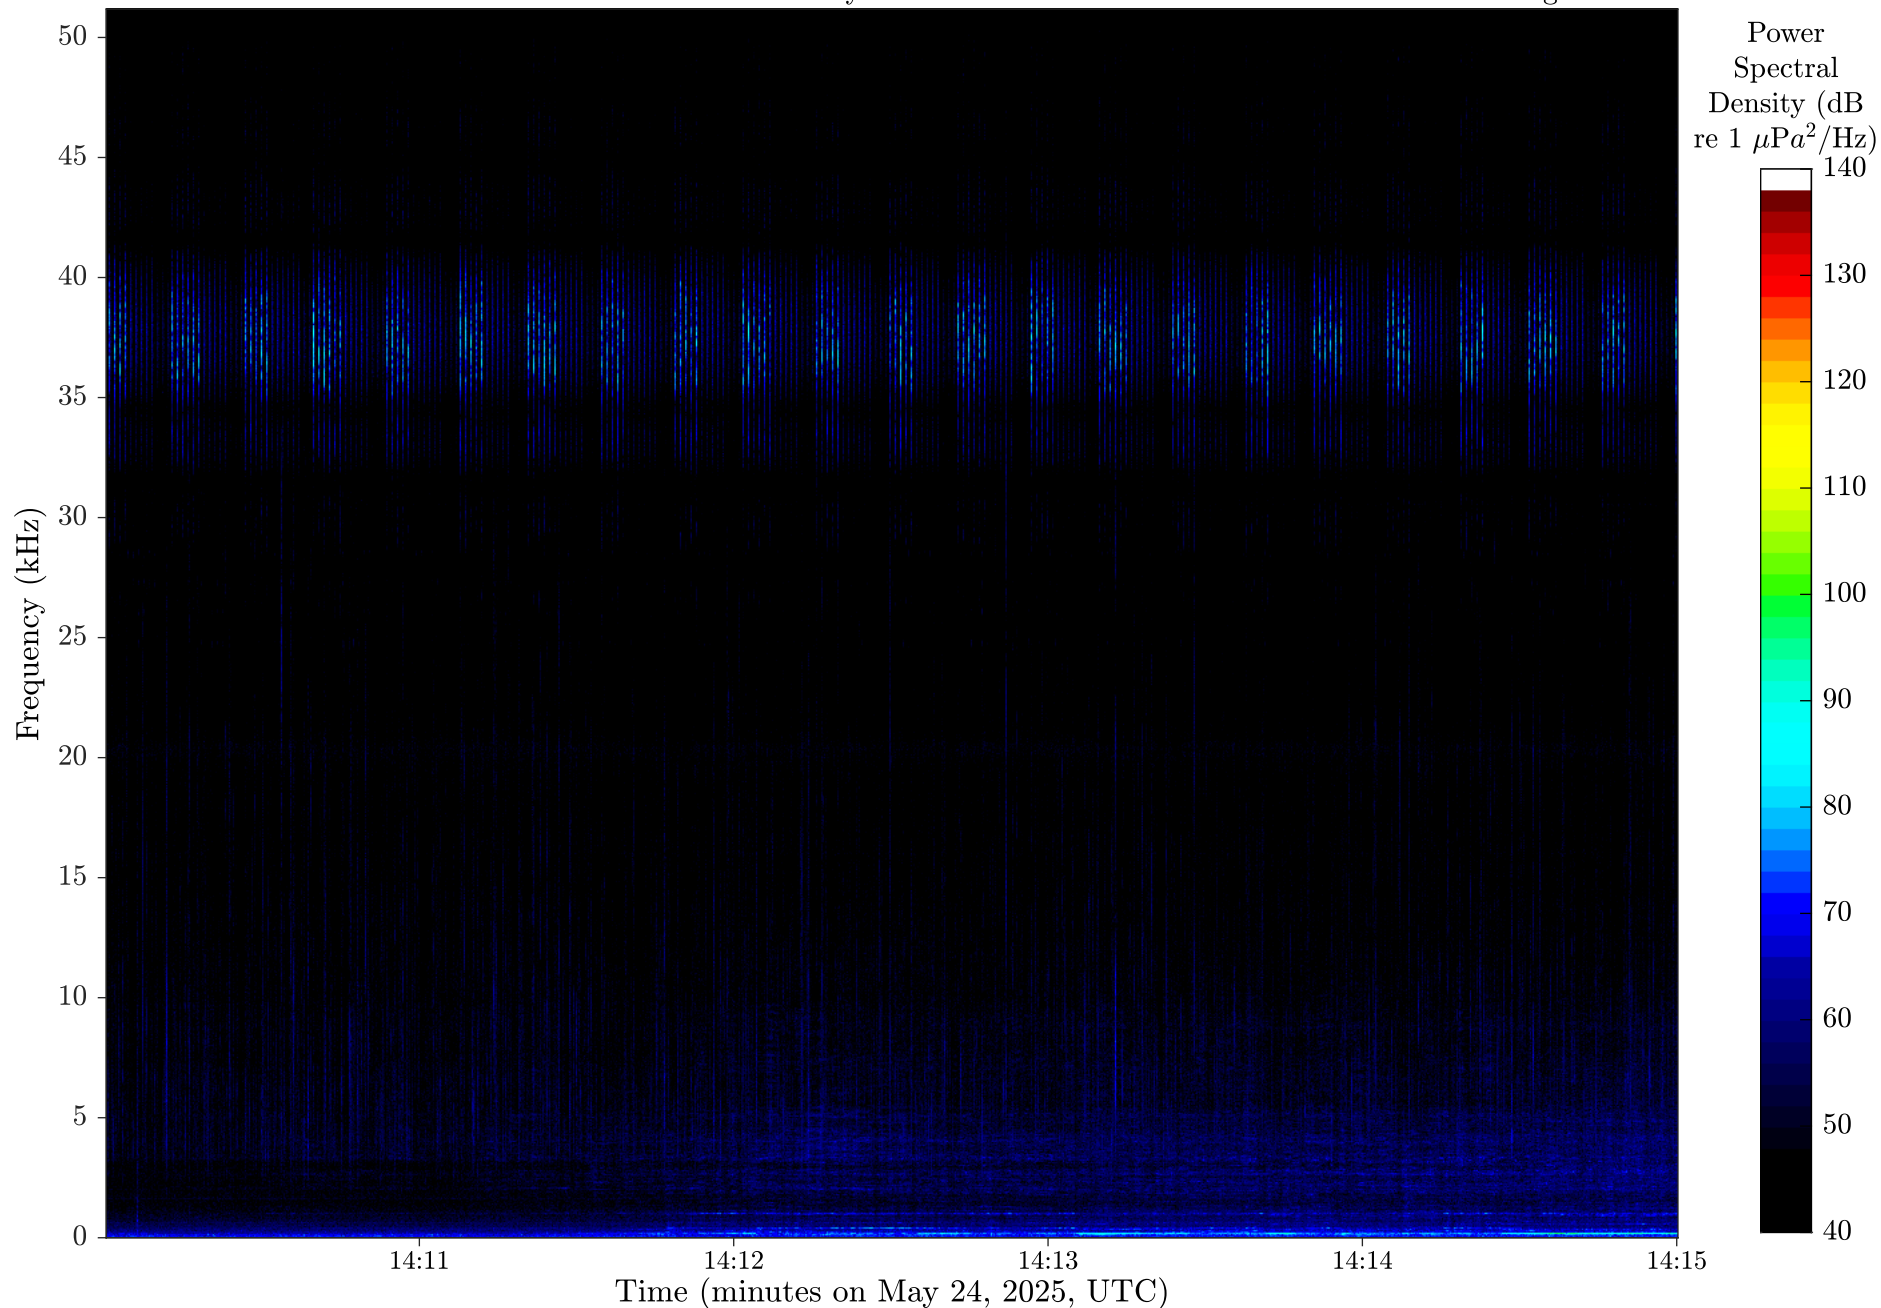


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:38:40 UTC

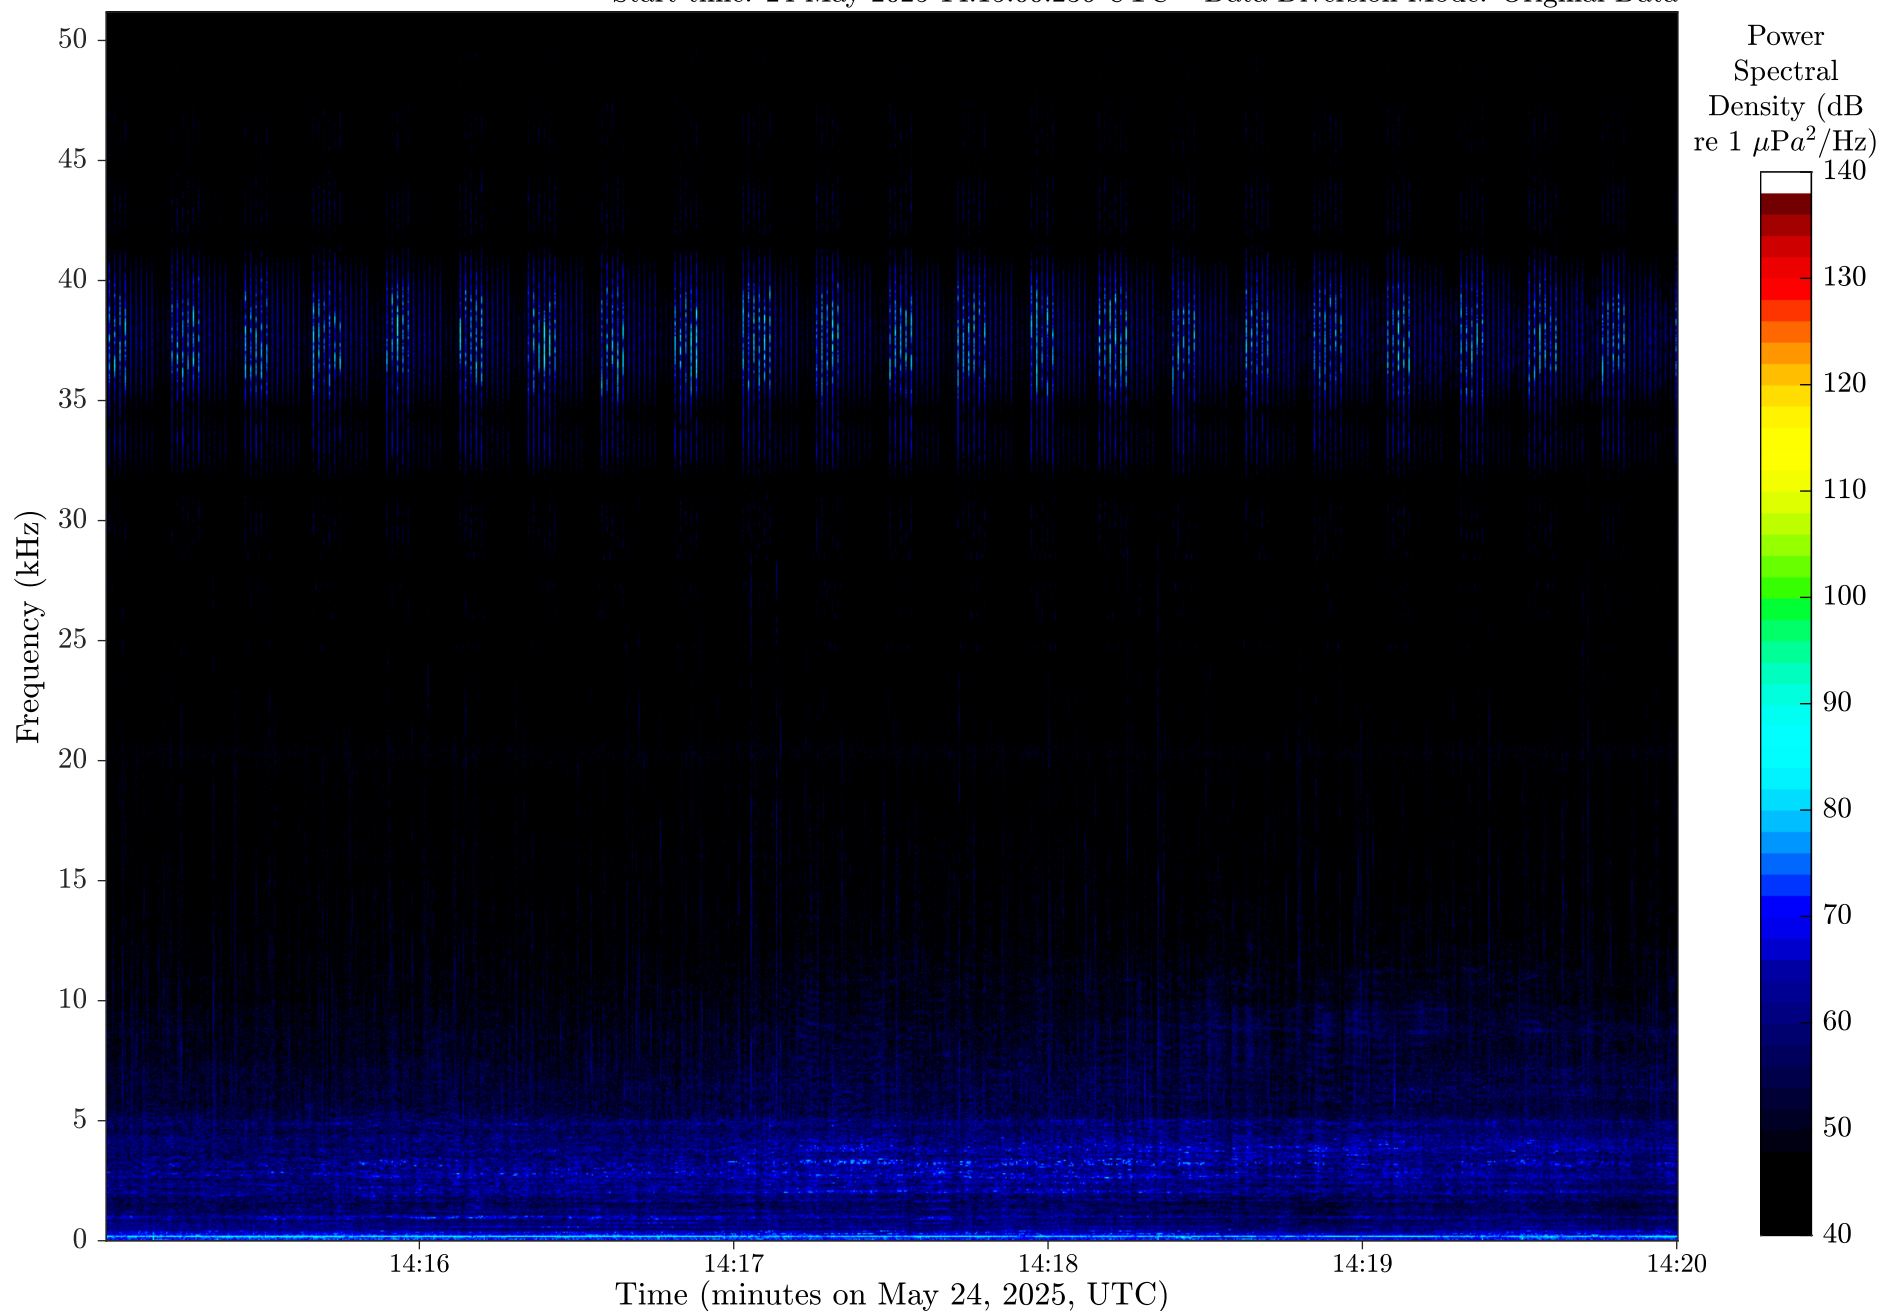

Comments: 31.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:38:48 UTC

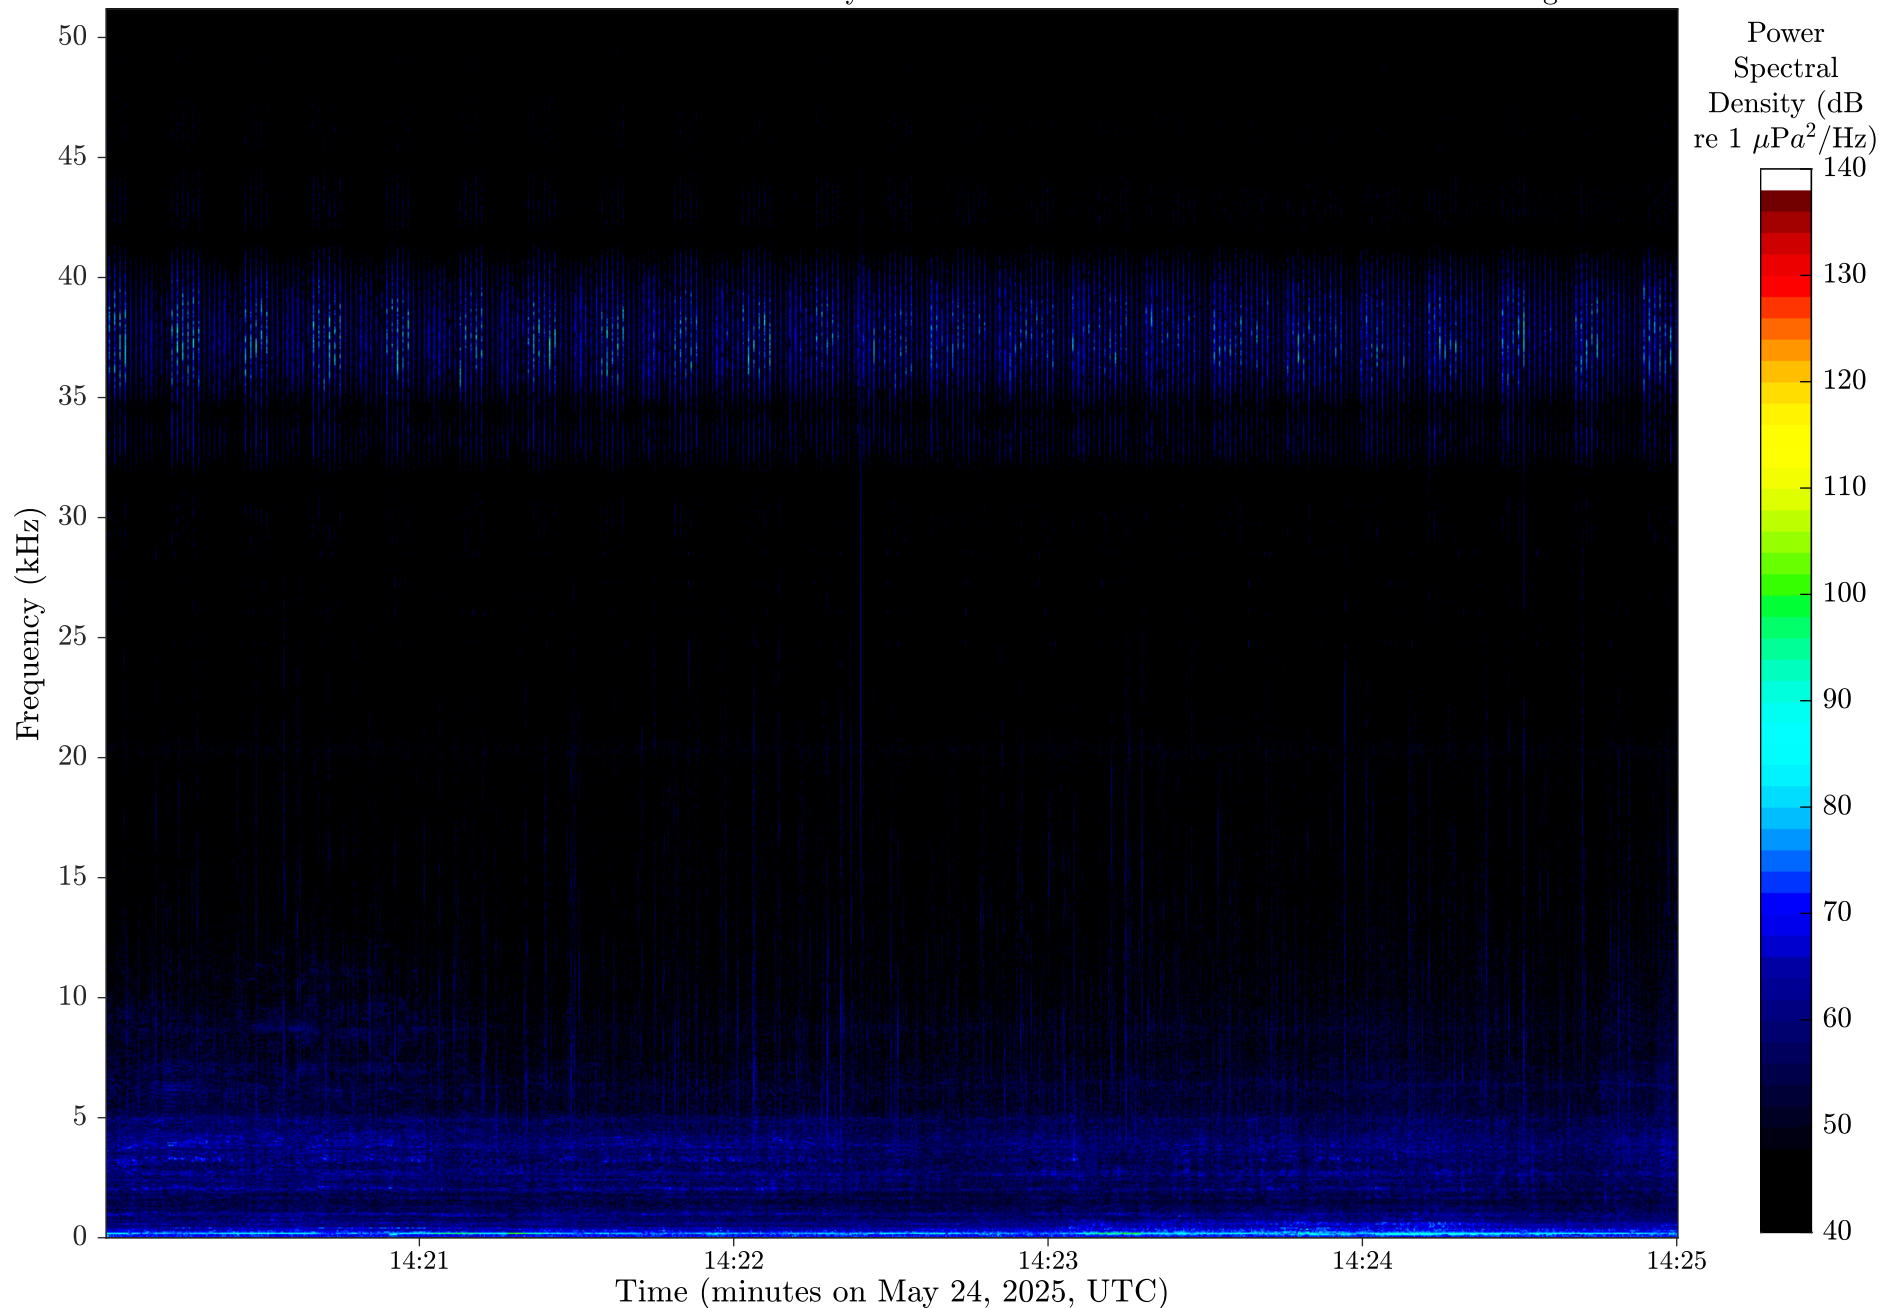

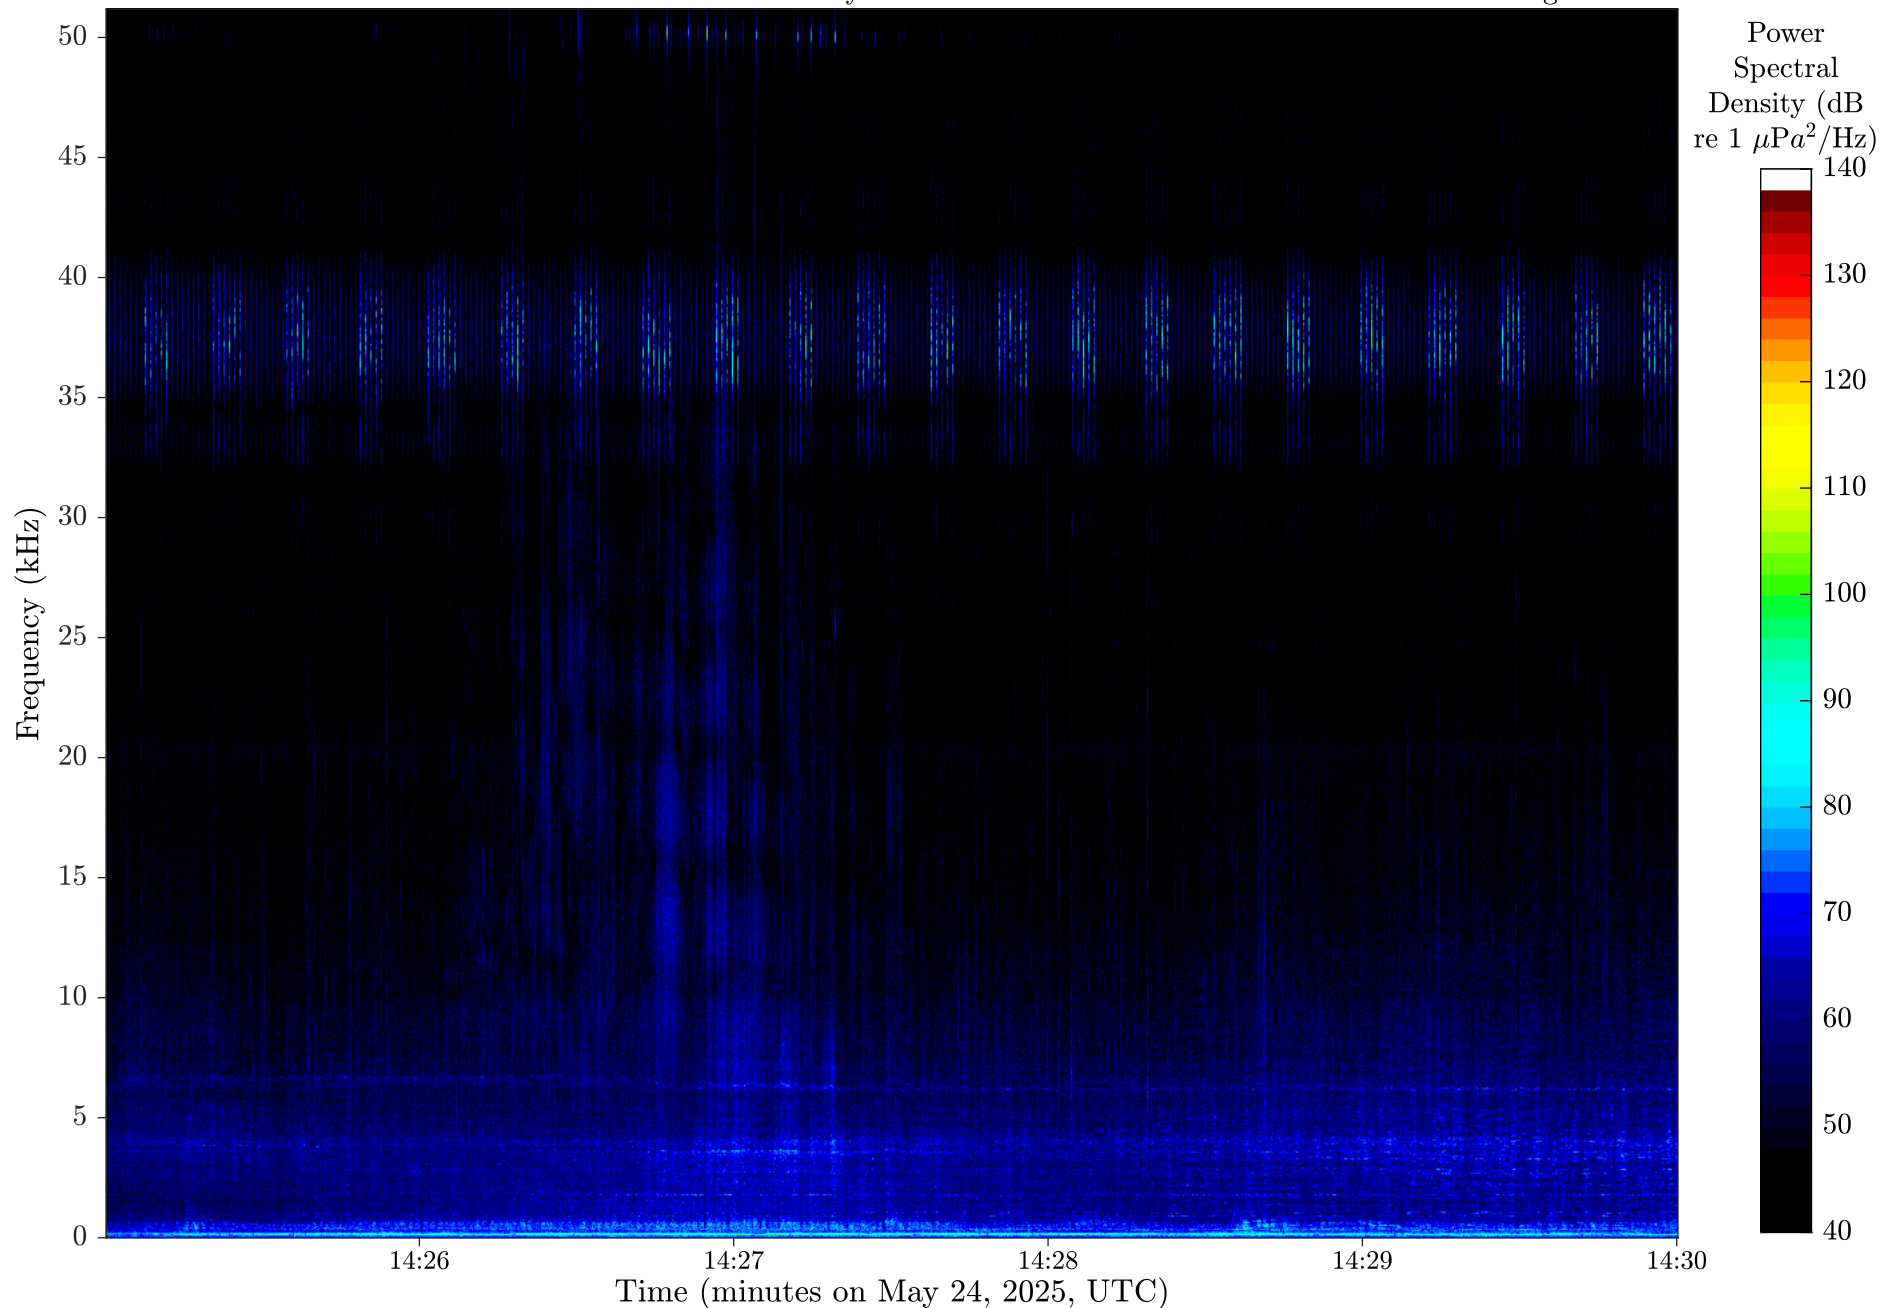


Comments: 20.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:05 UTC

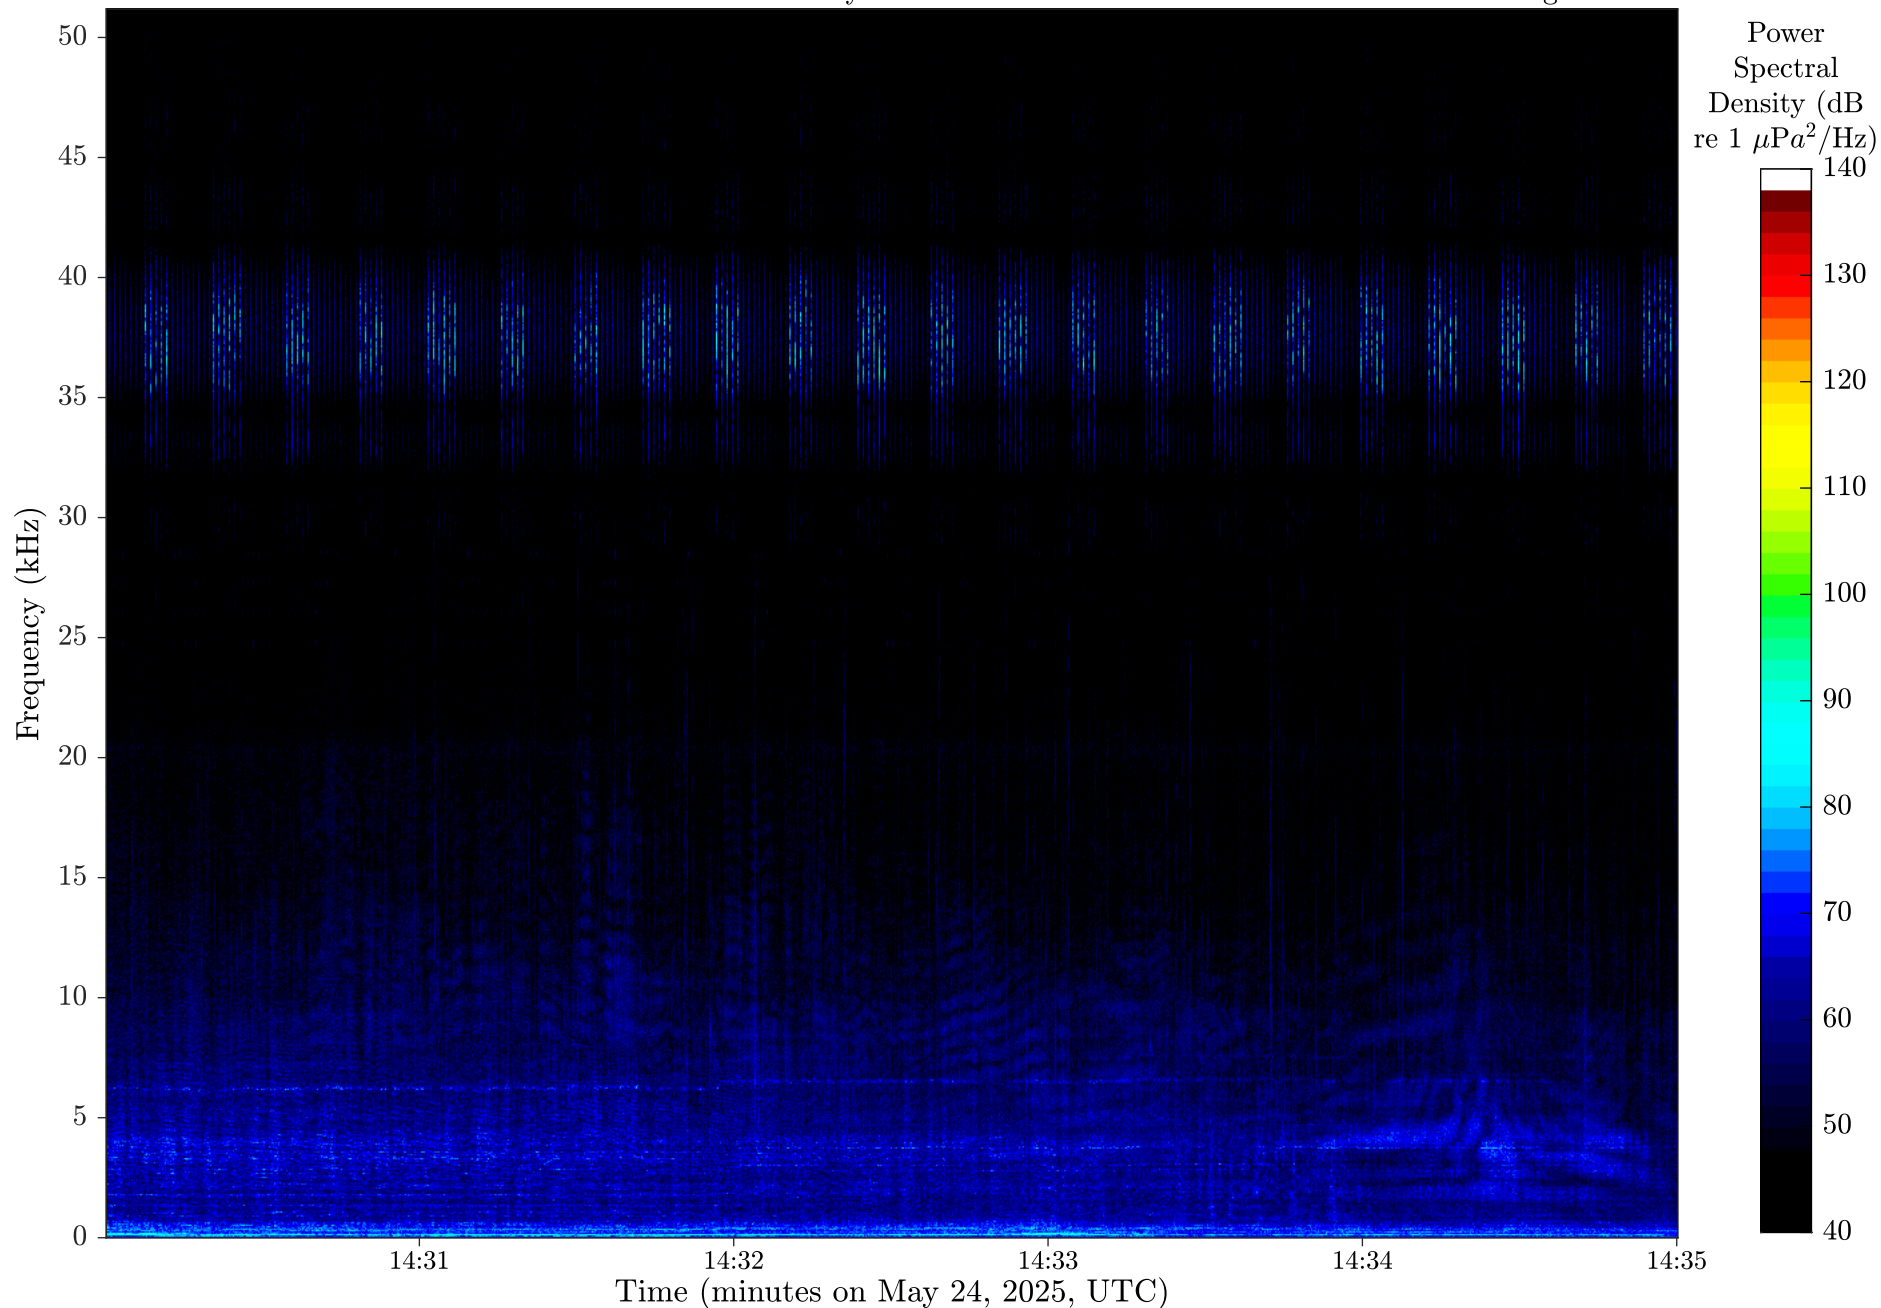


Comments: 27.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:13 UTC

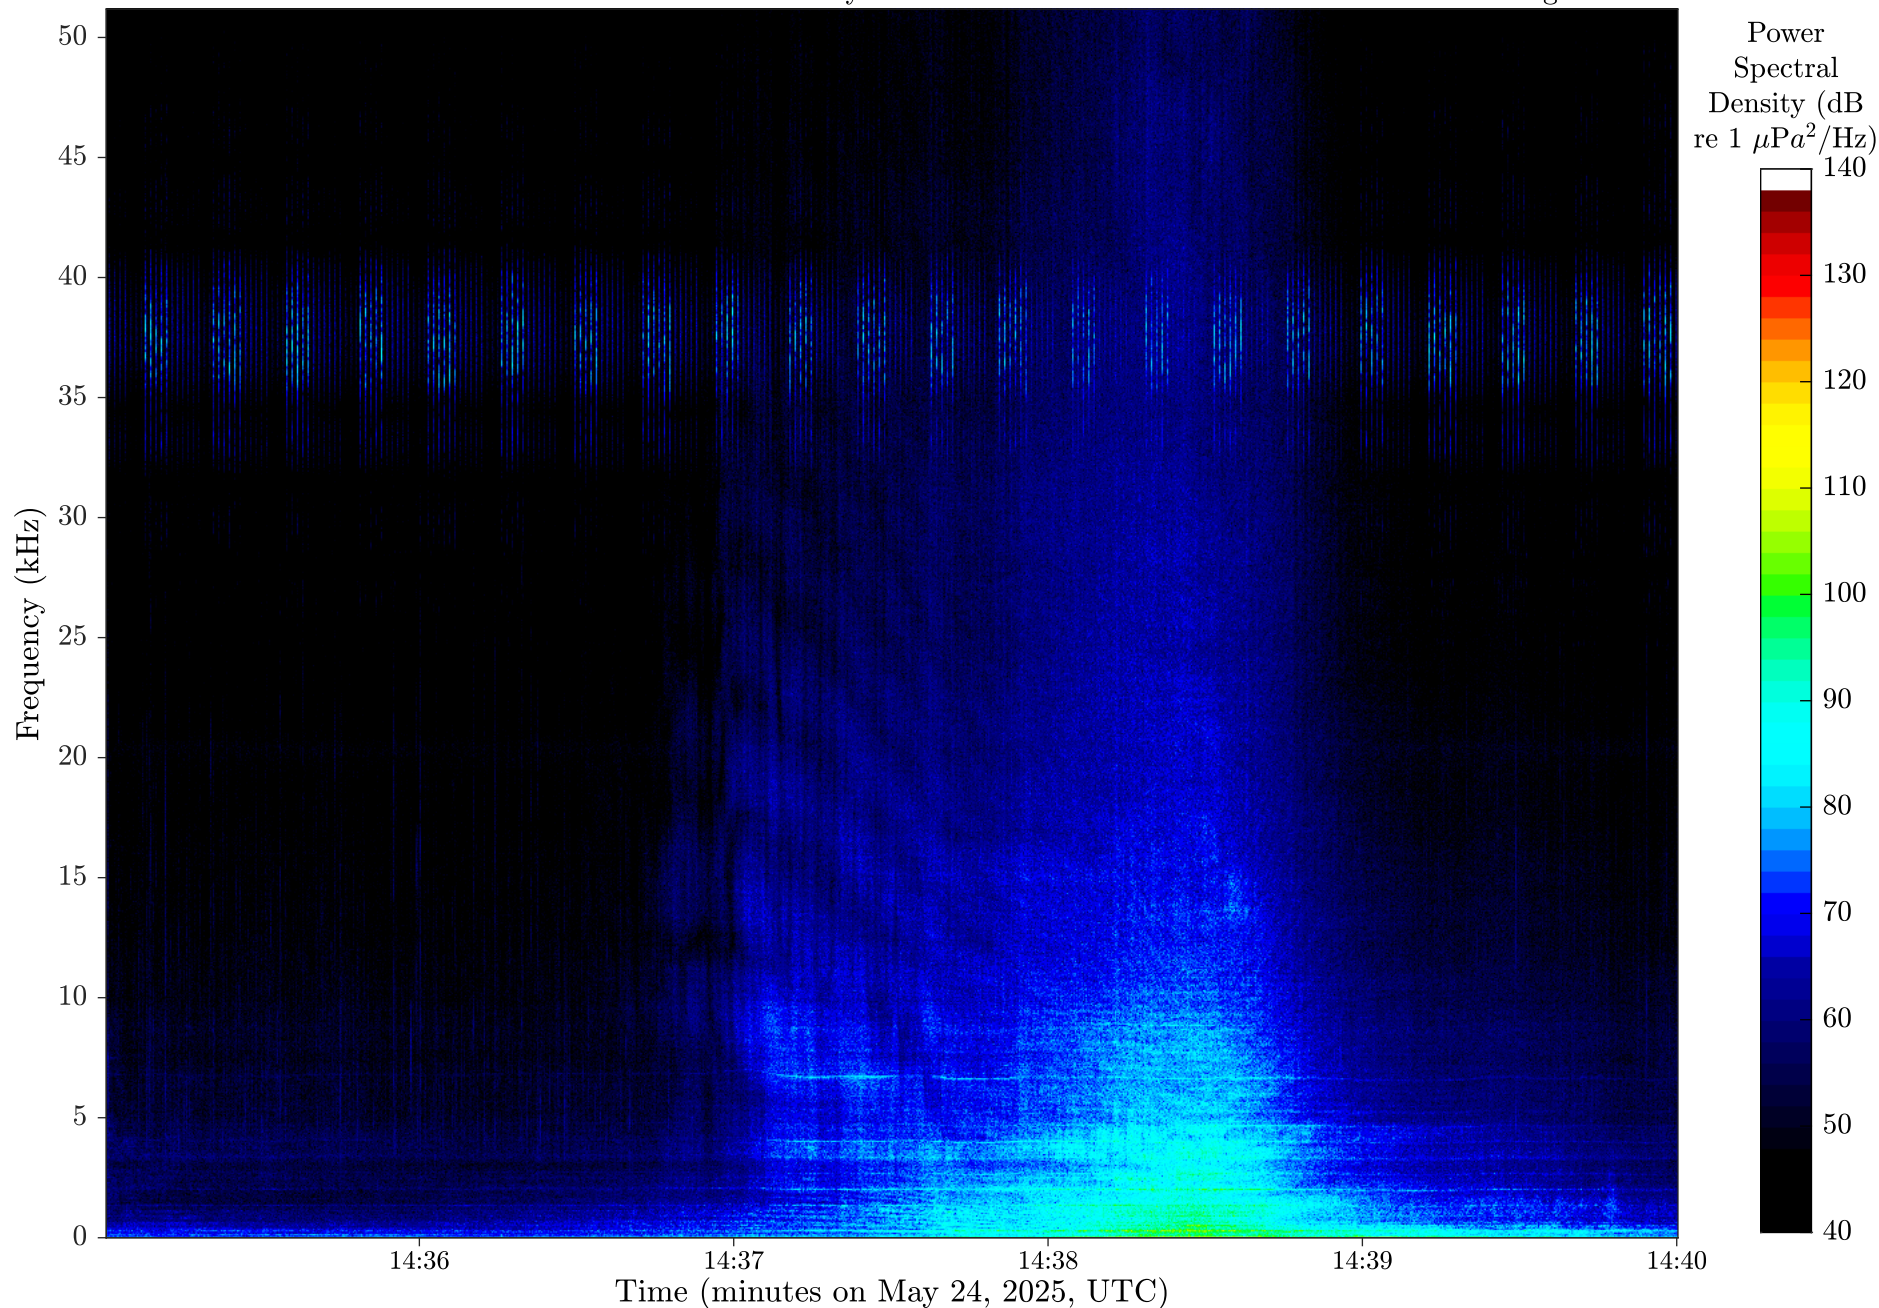


Comments: 15 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:39:21 UTC

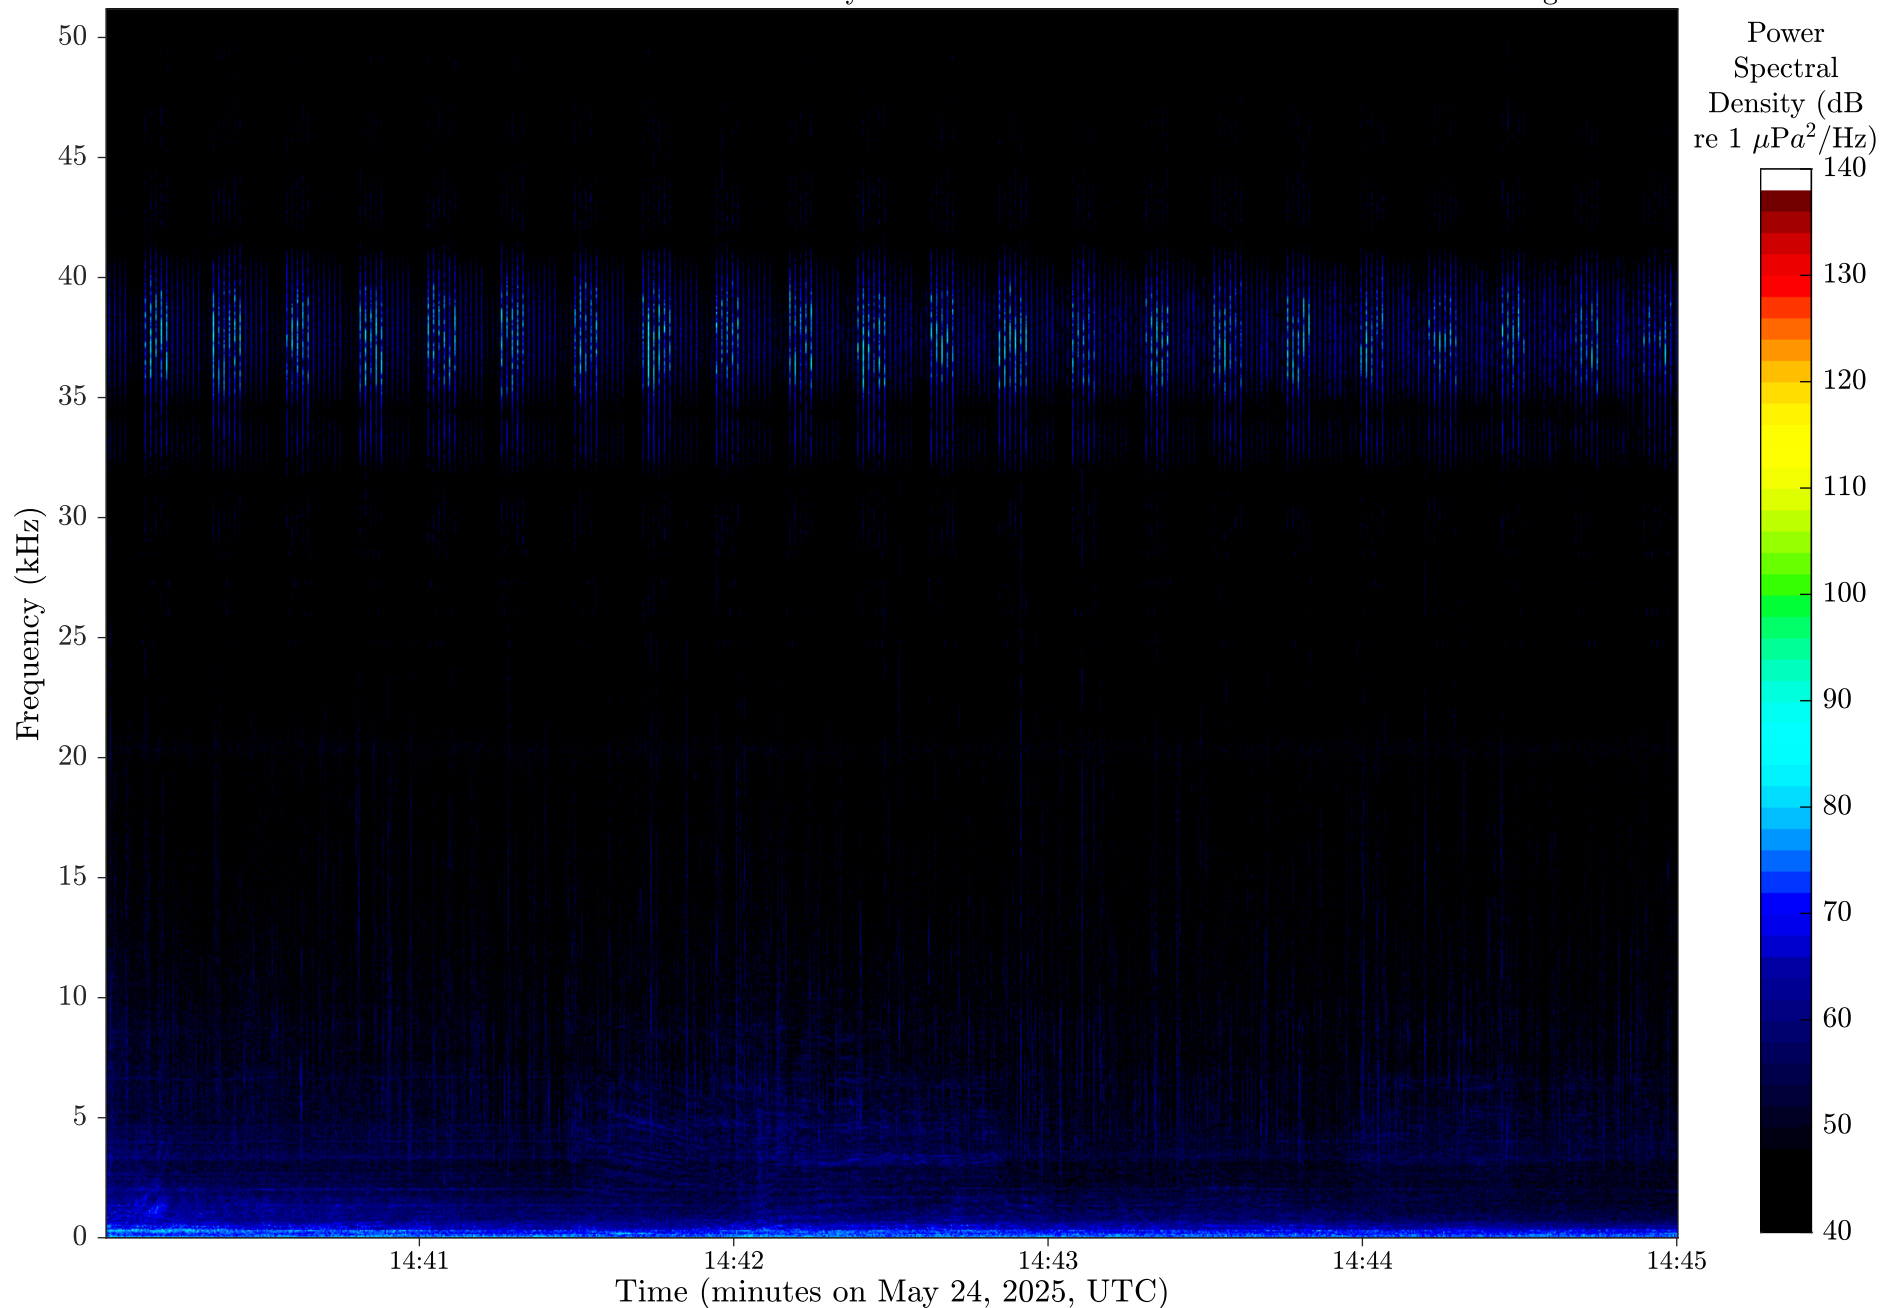

Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:39:30 UTC

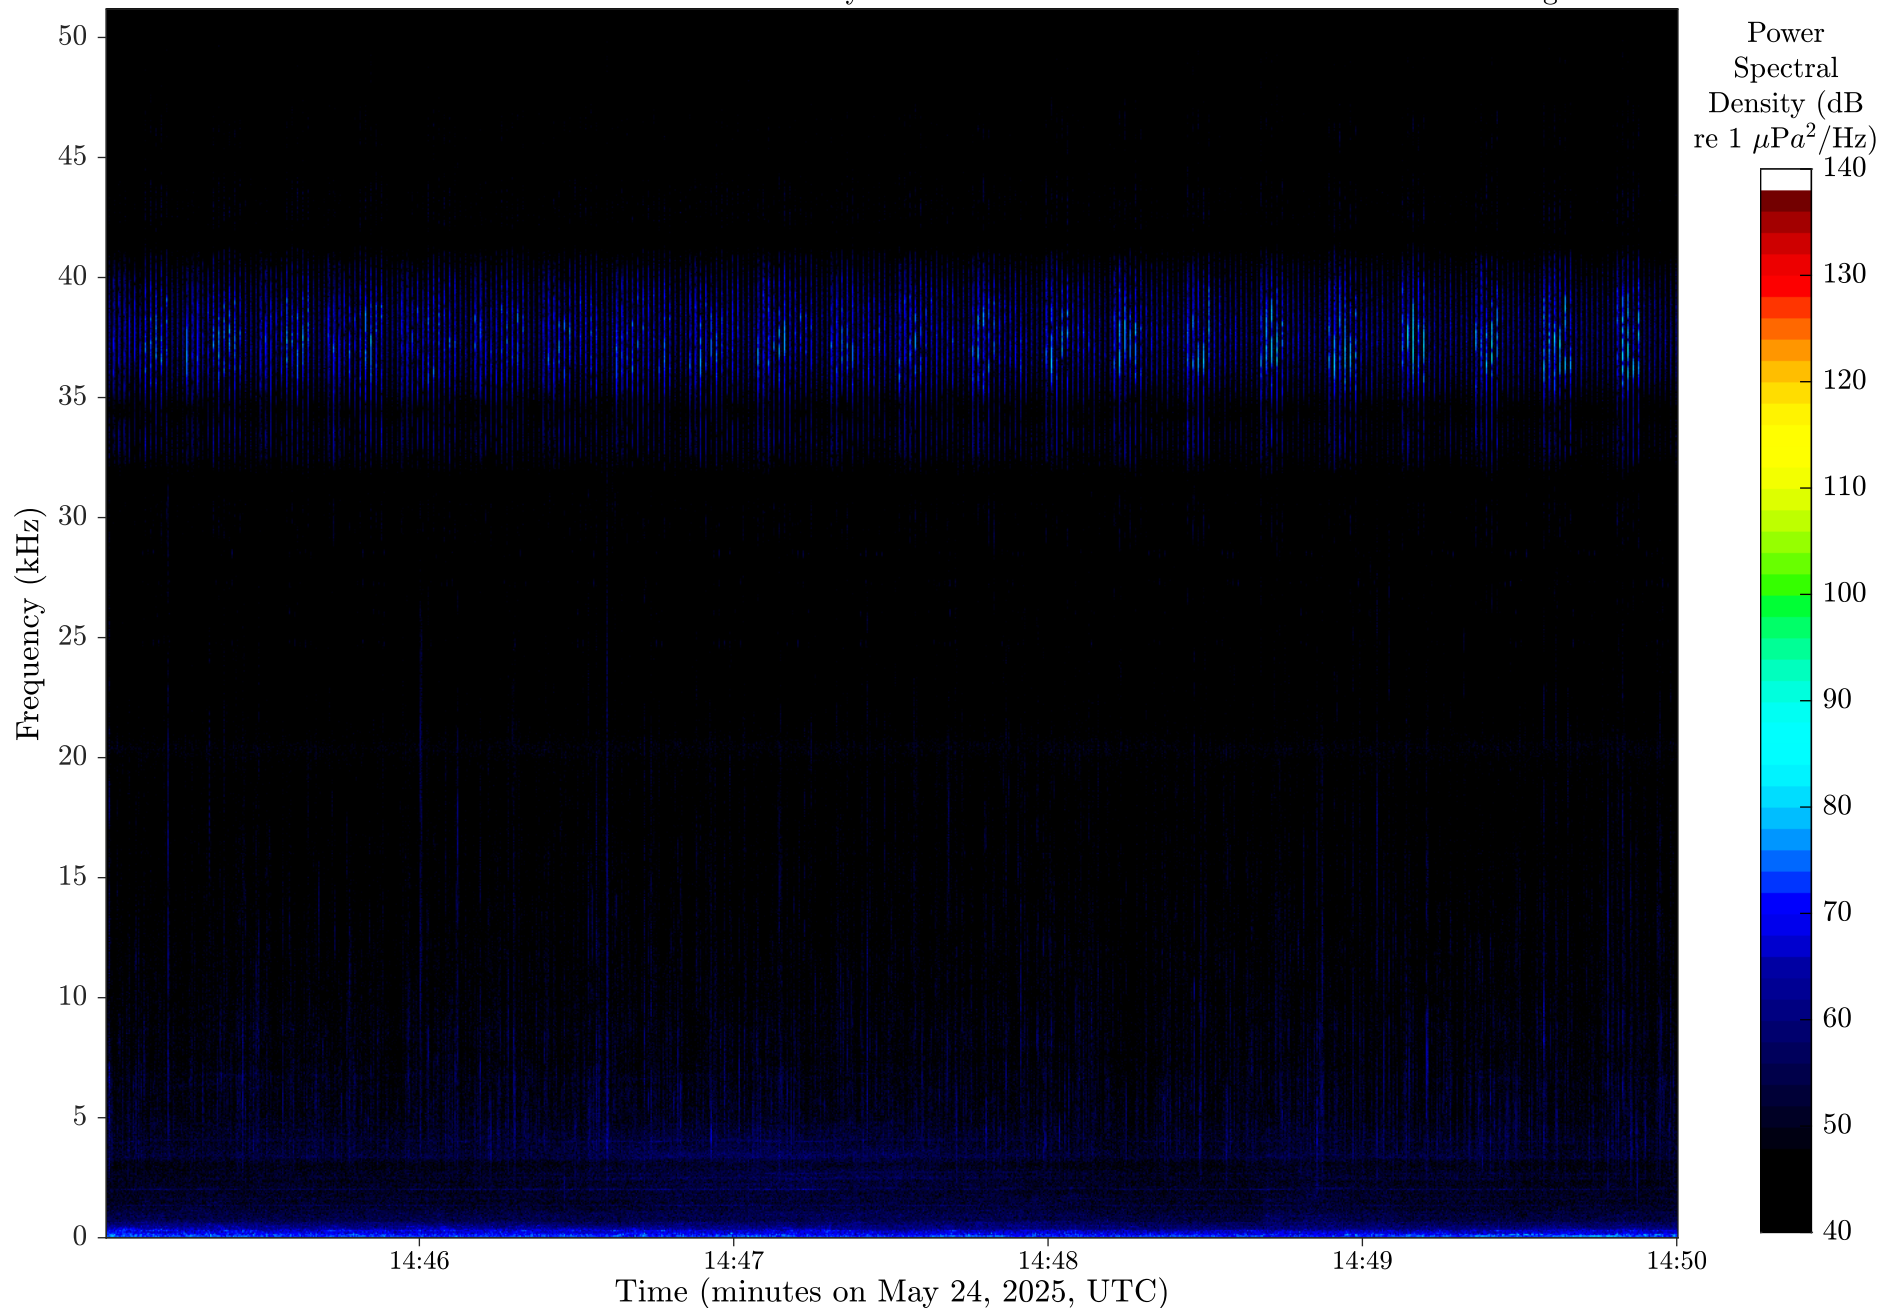


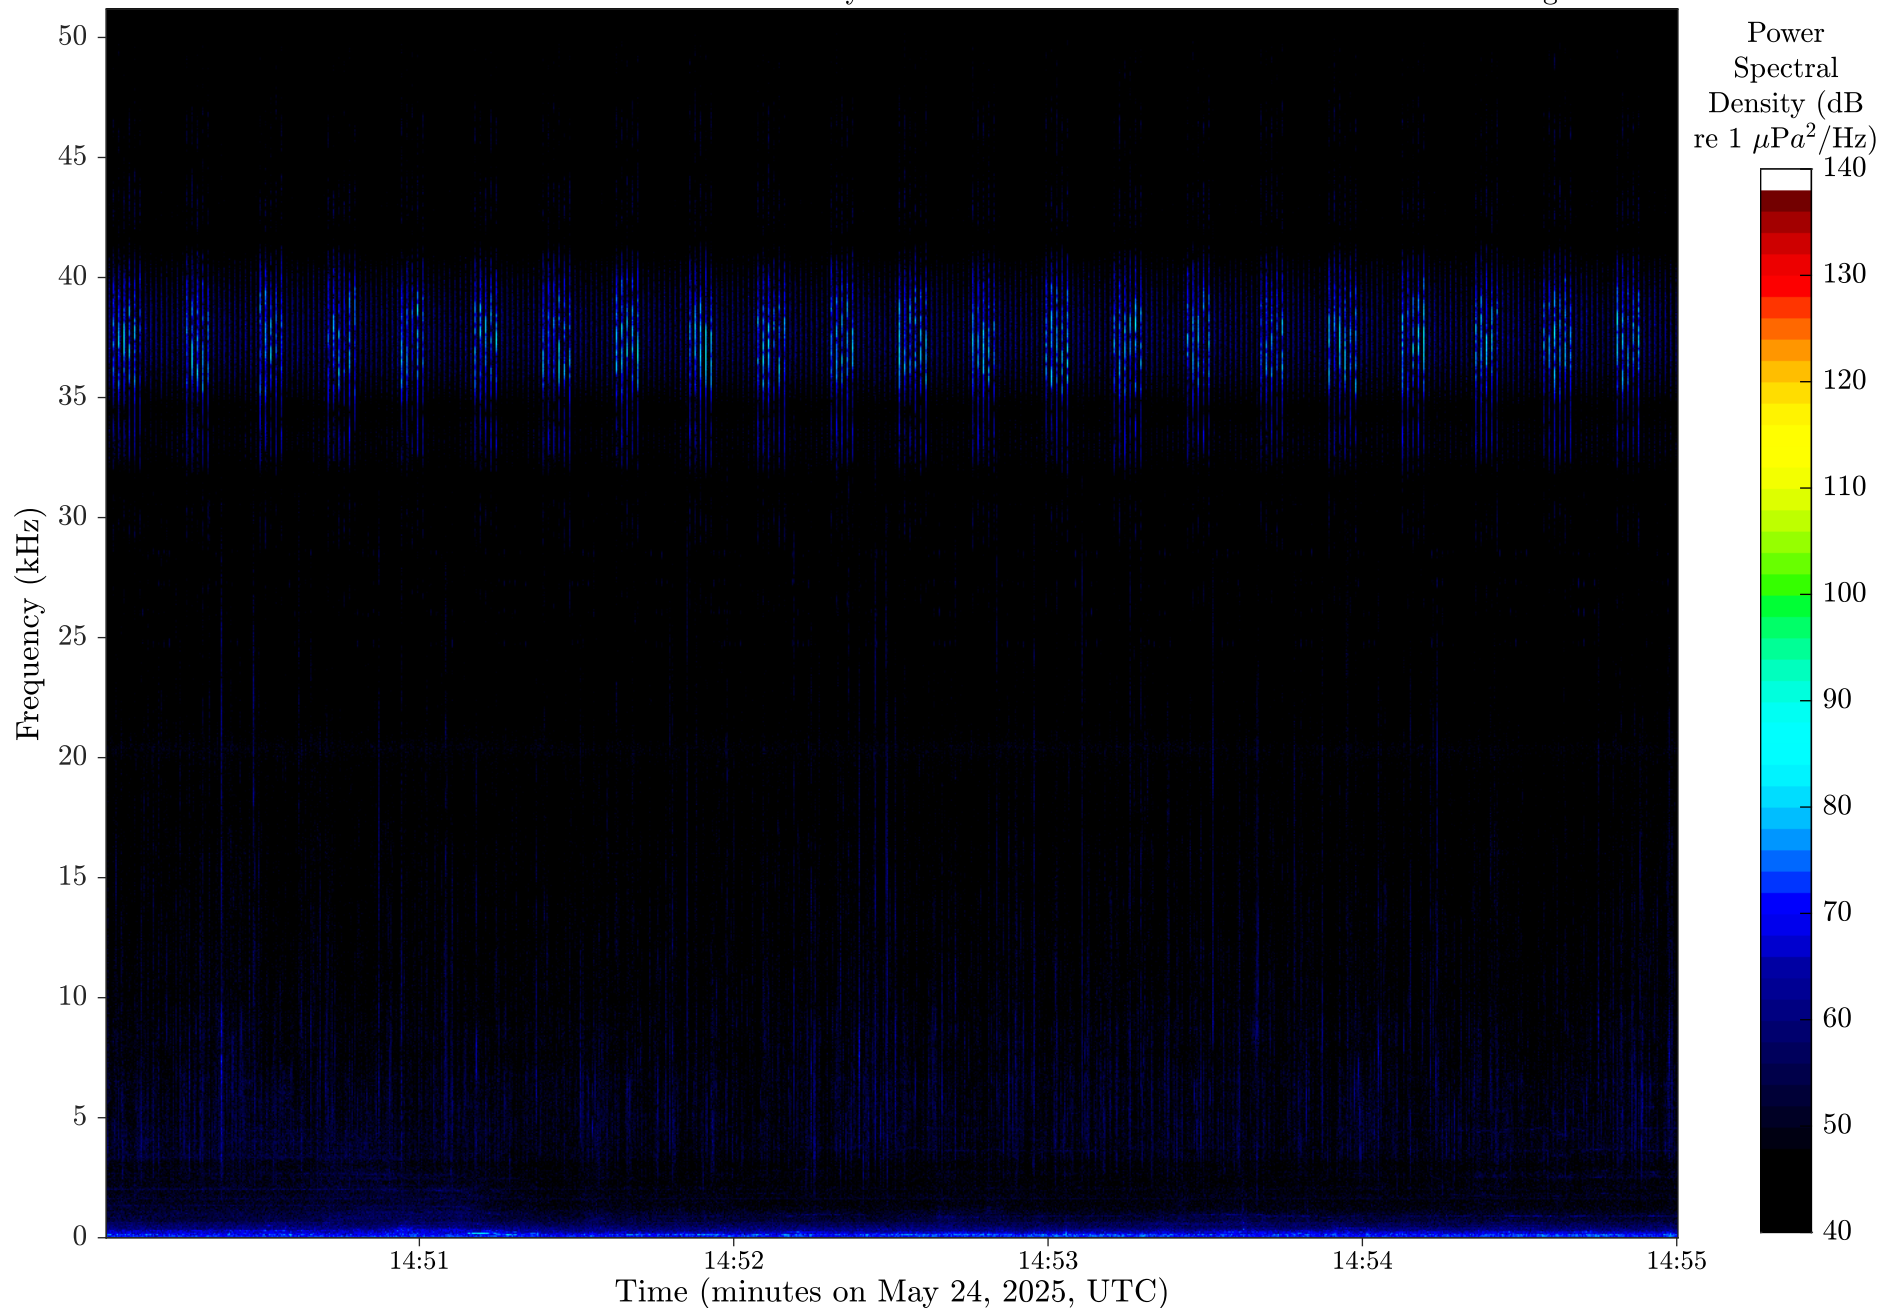

Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:39:46 UTC

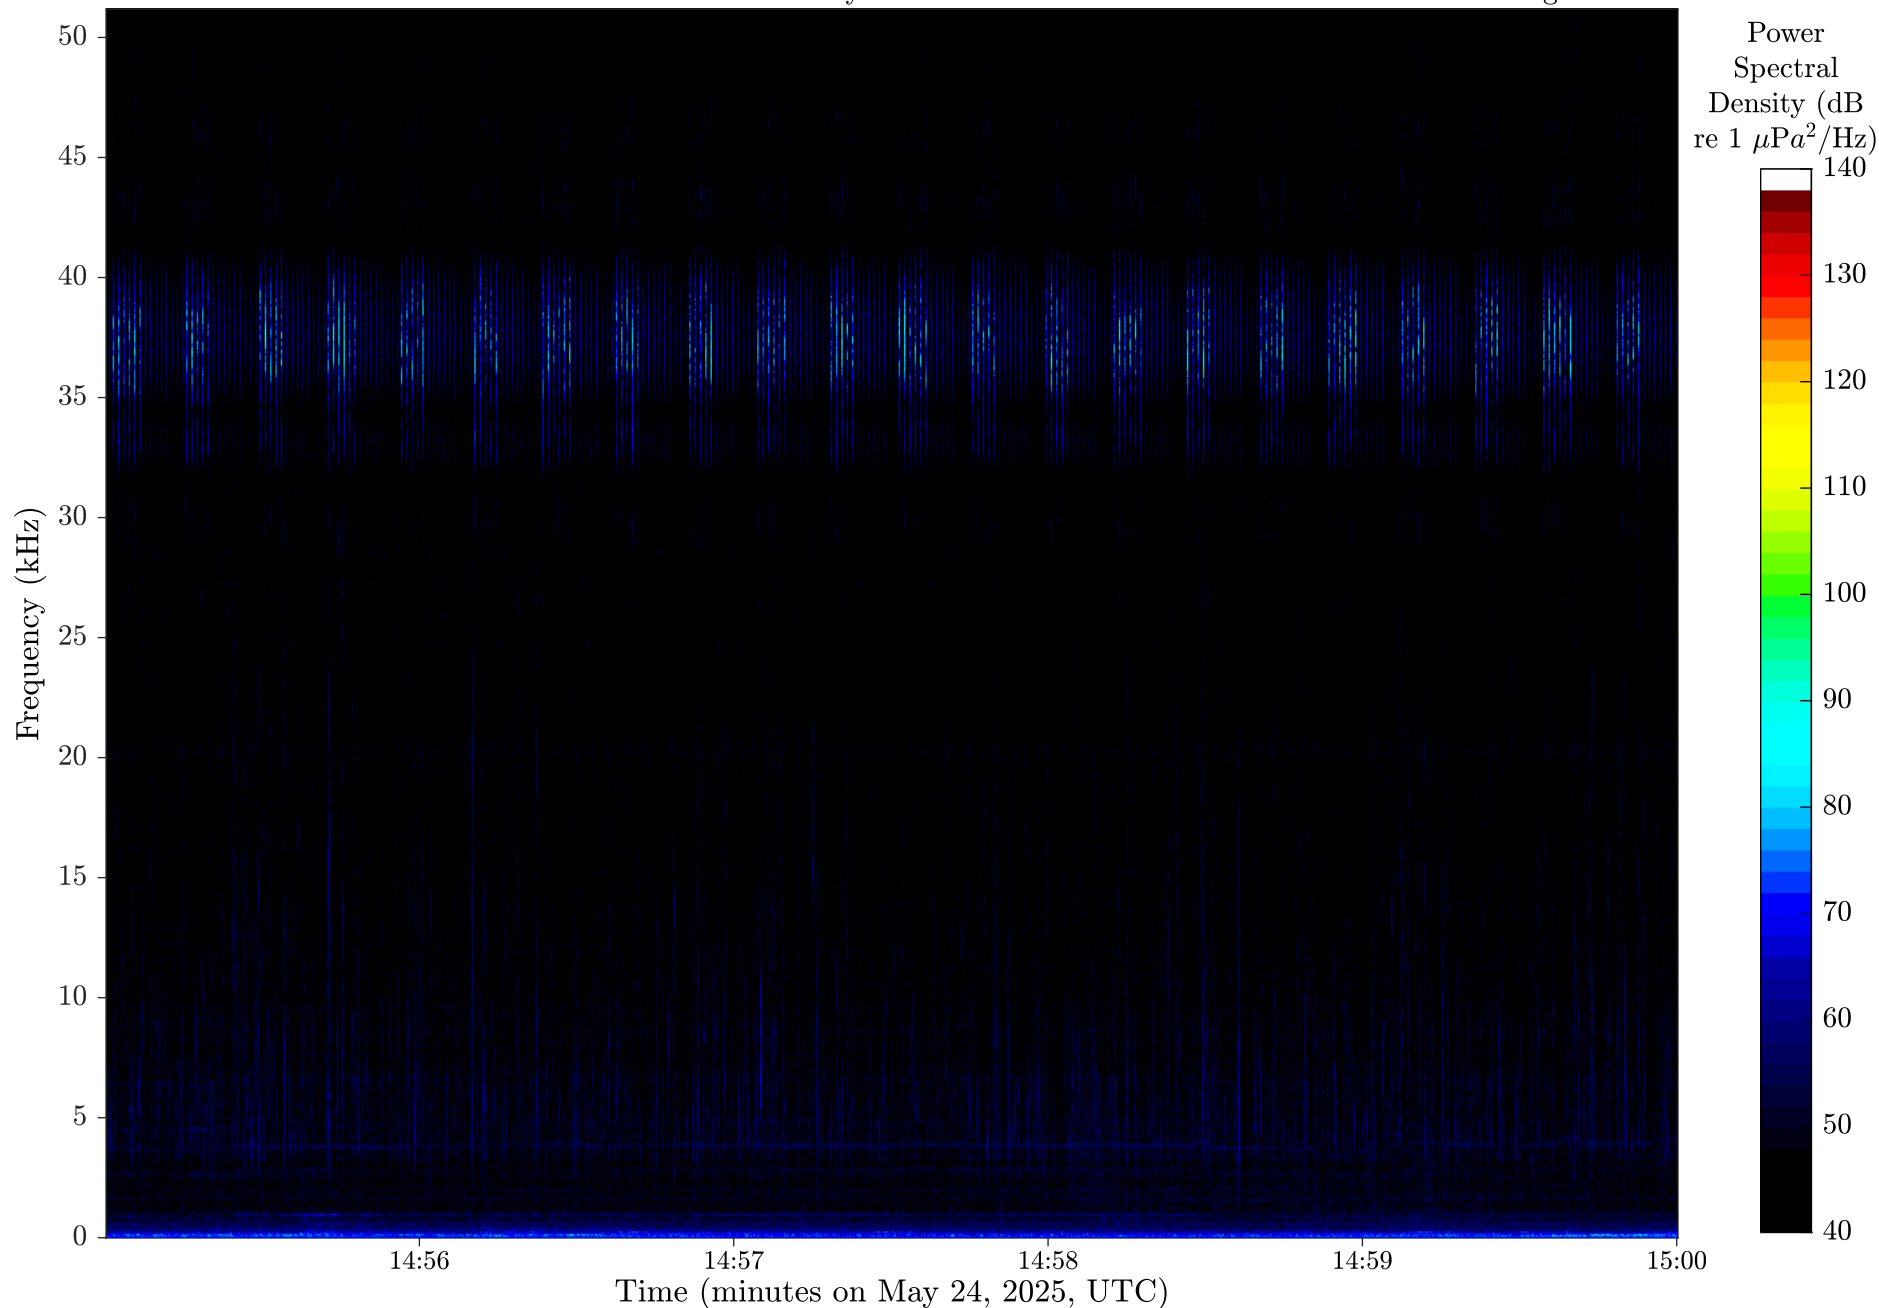

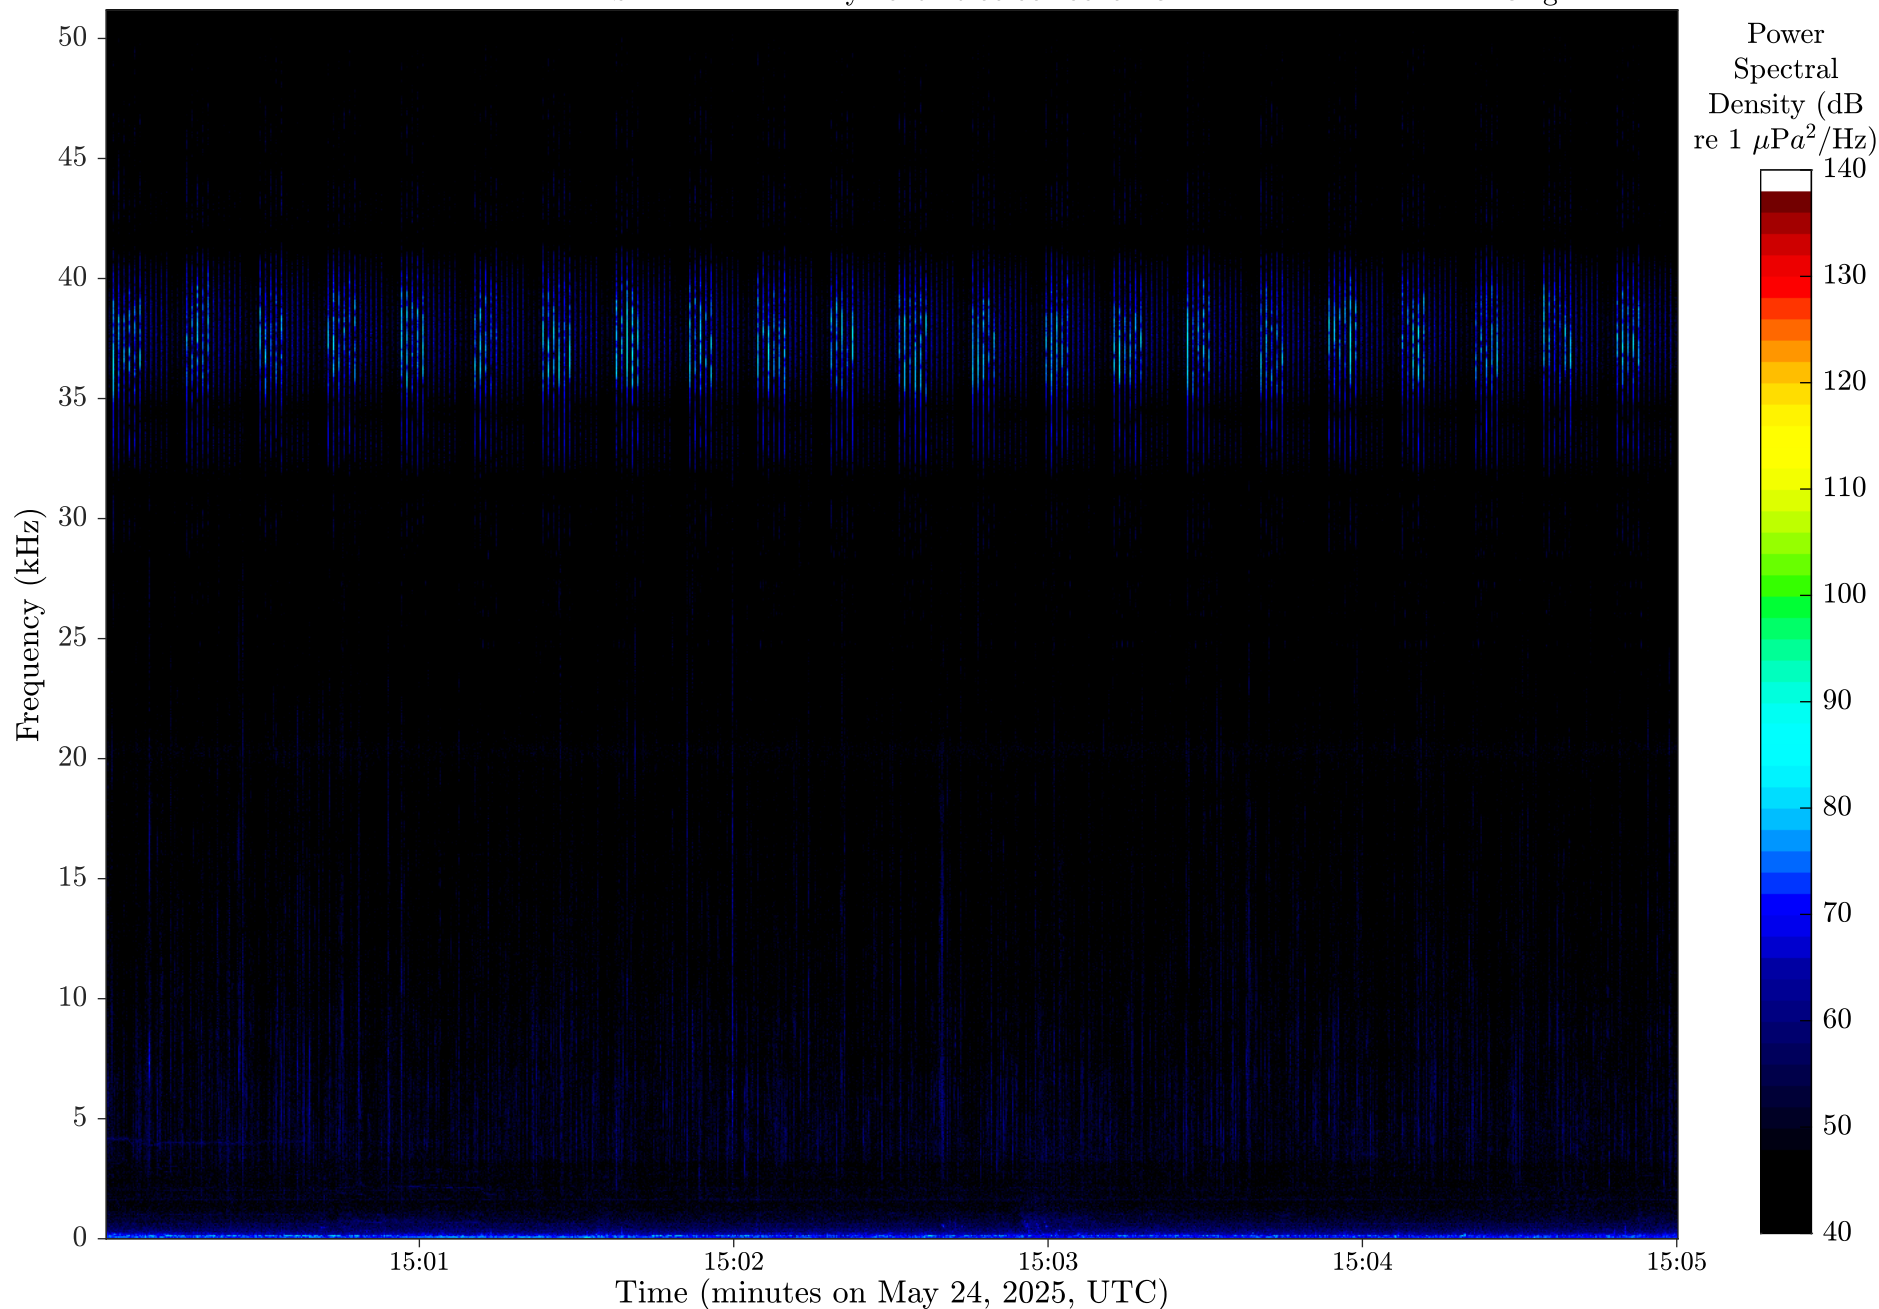


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:40:02 UTC

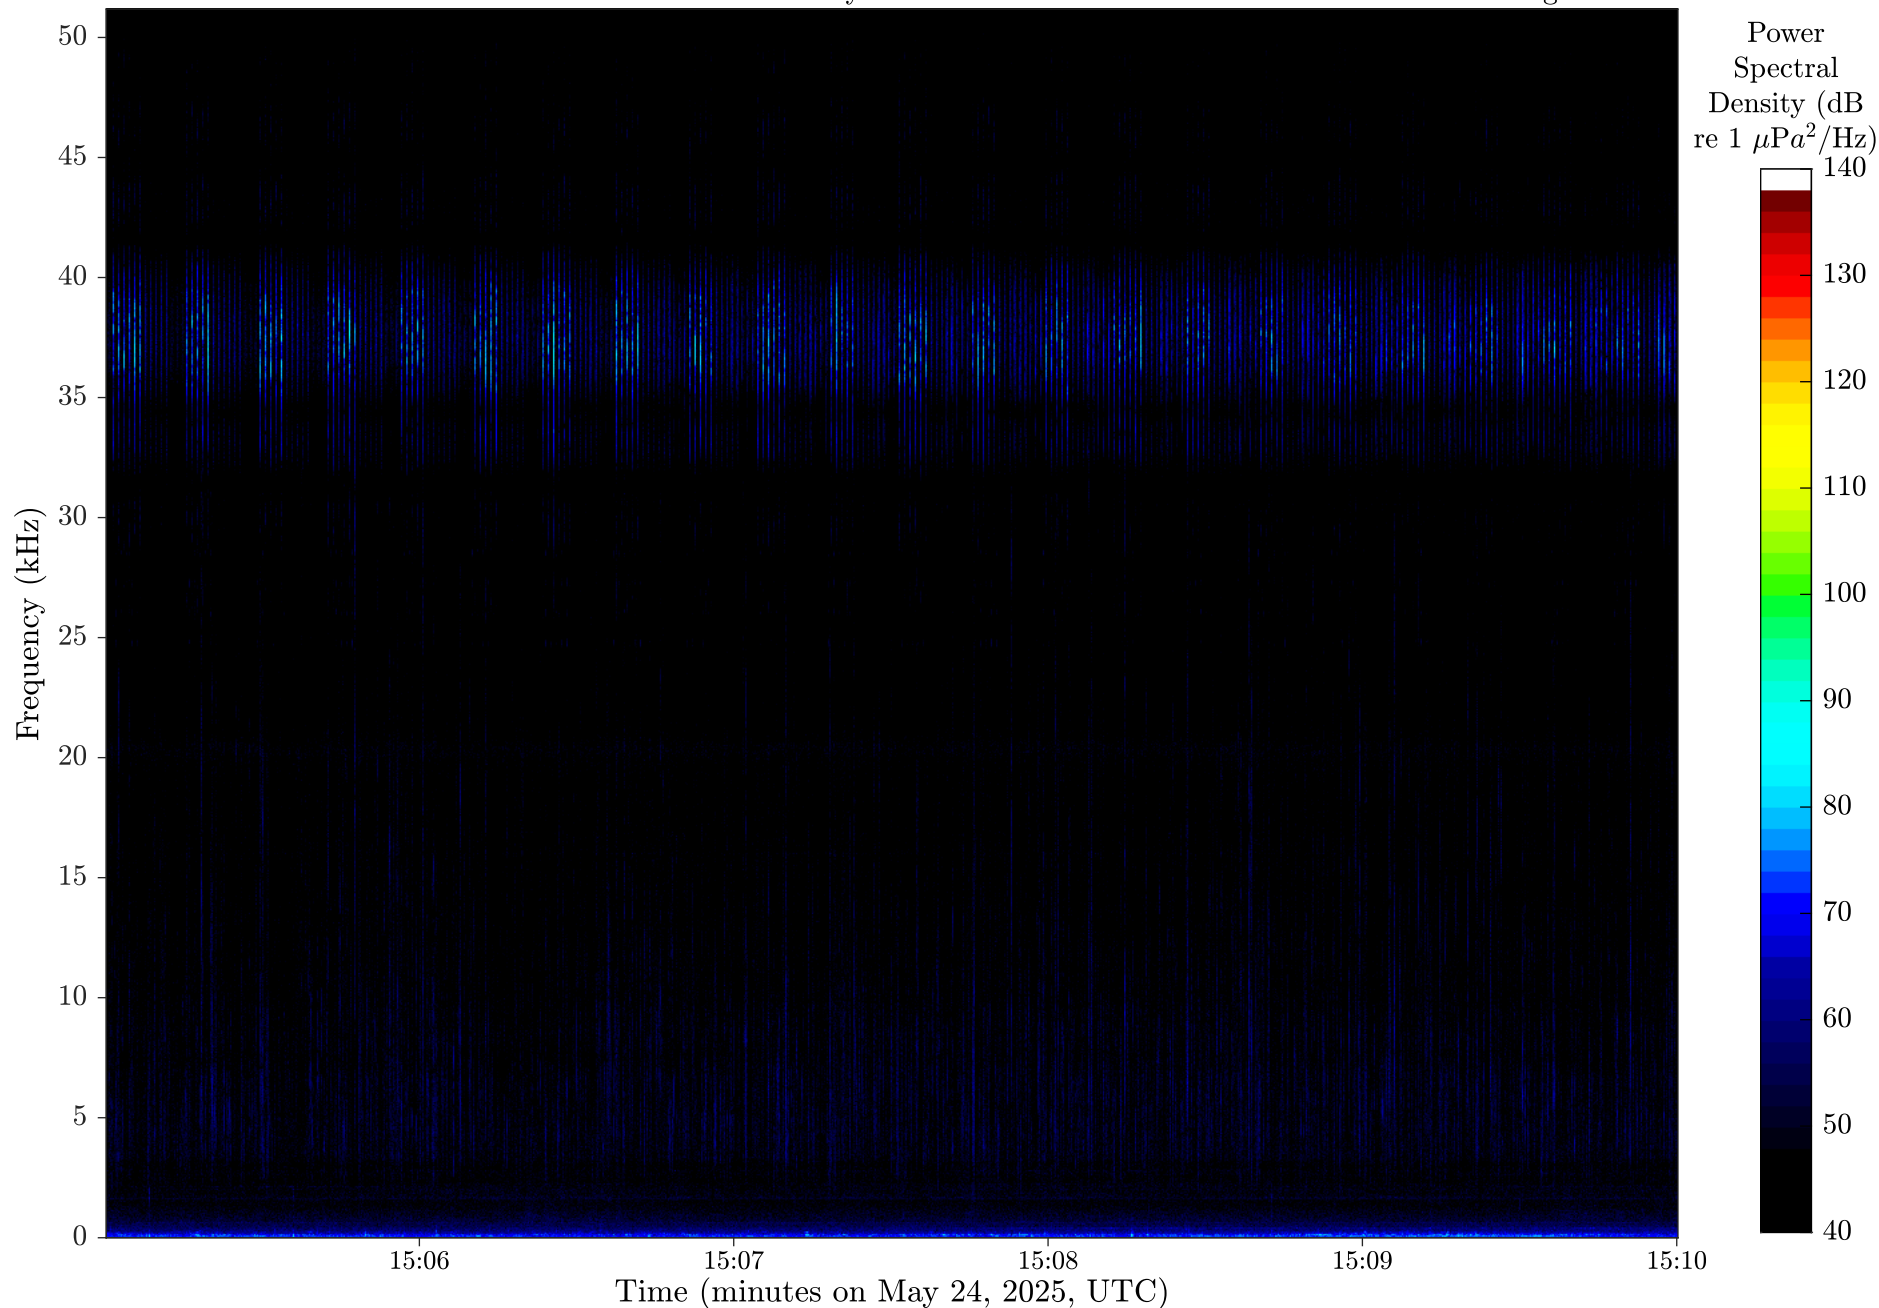

Comments: 32.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:40:11 UTC

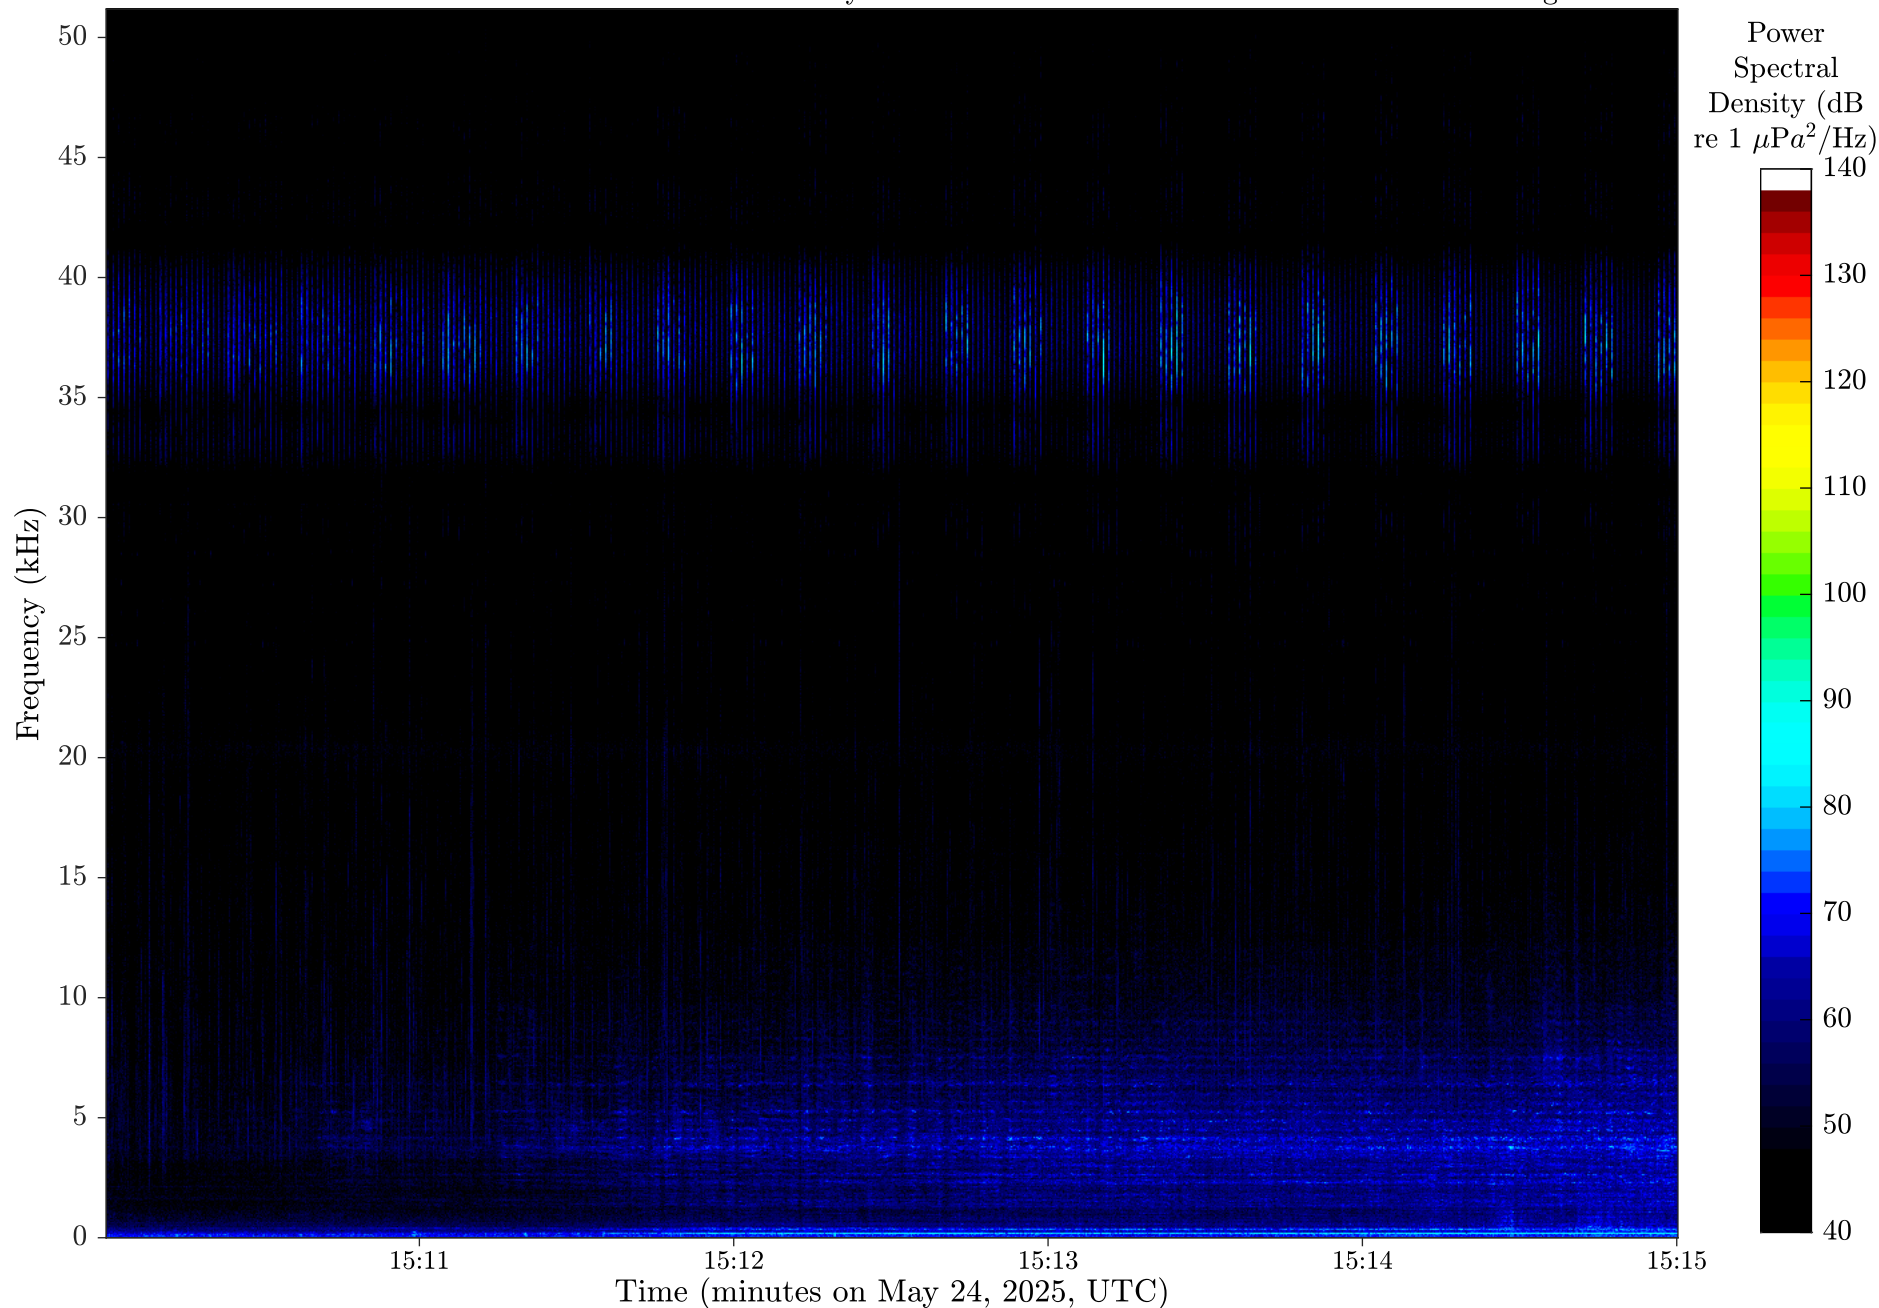

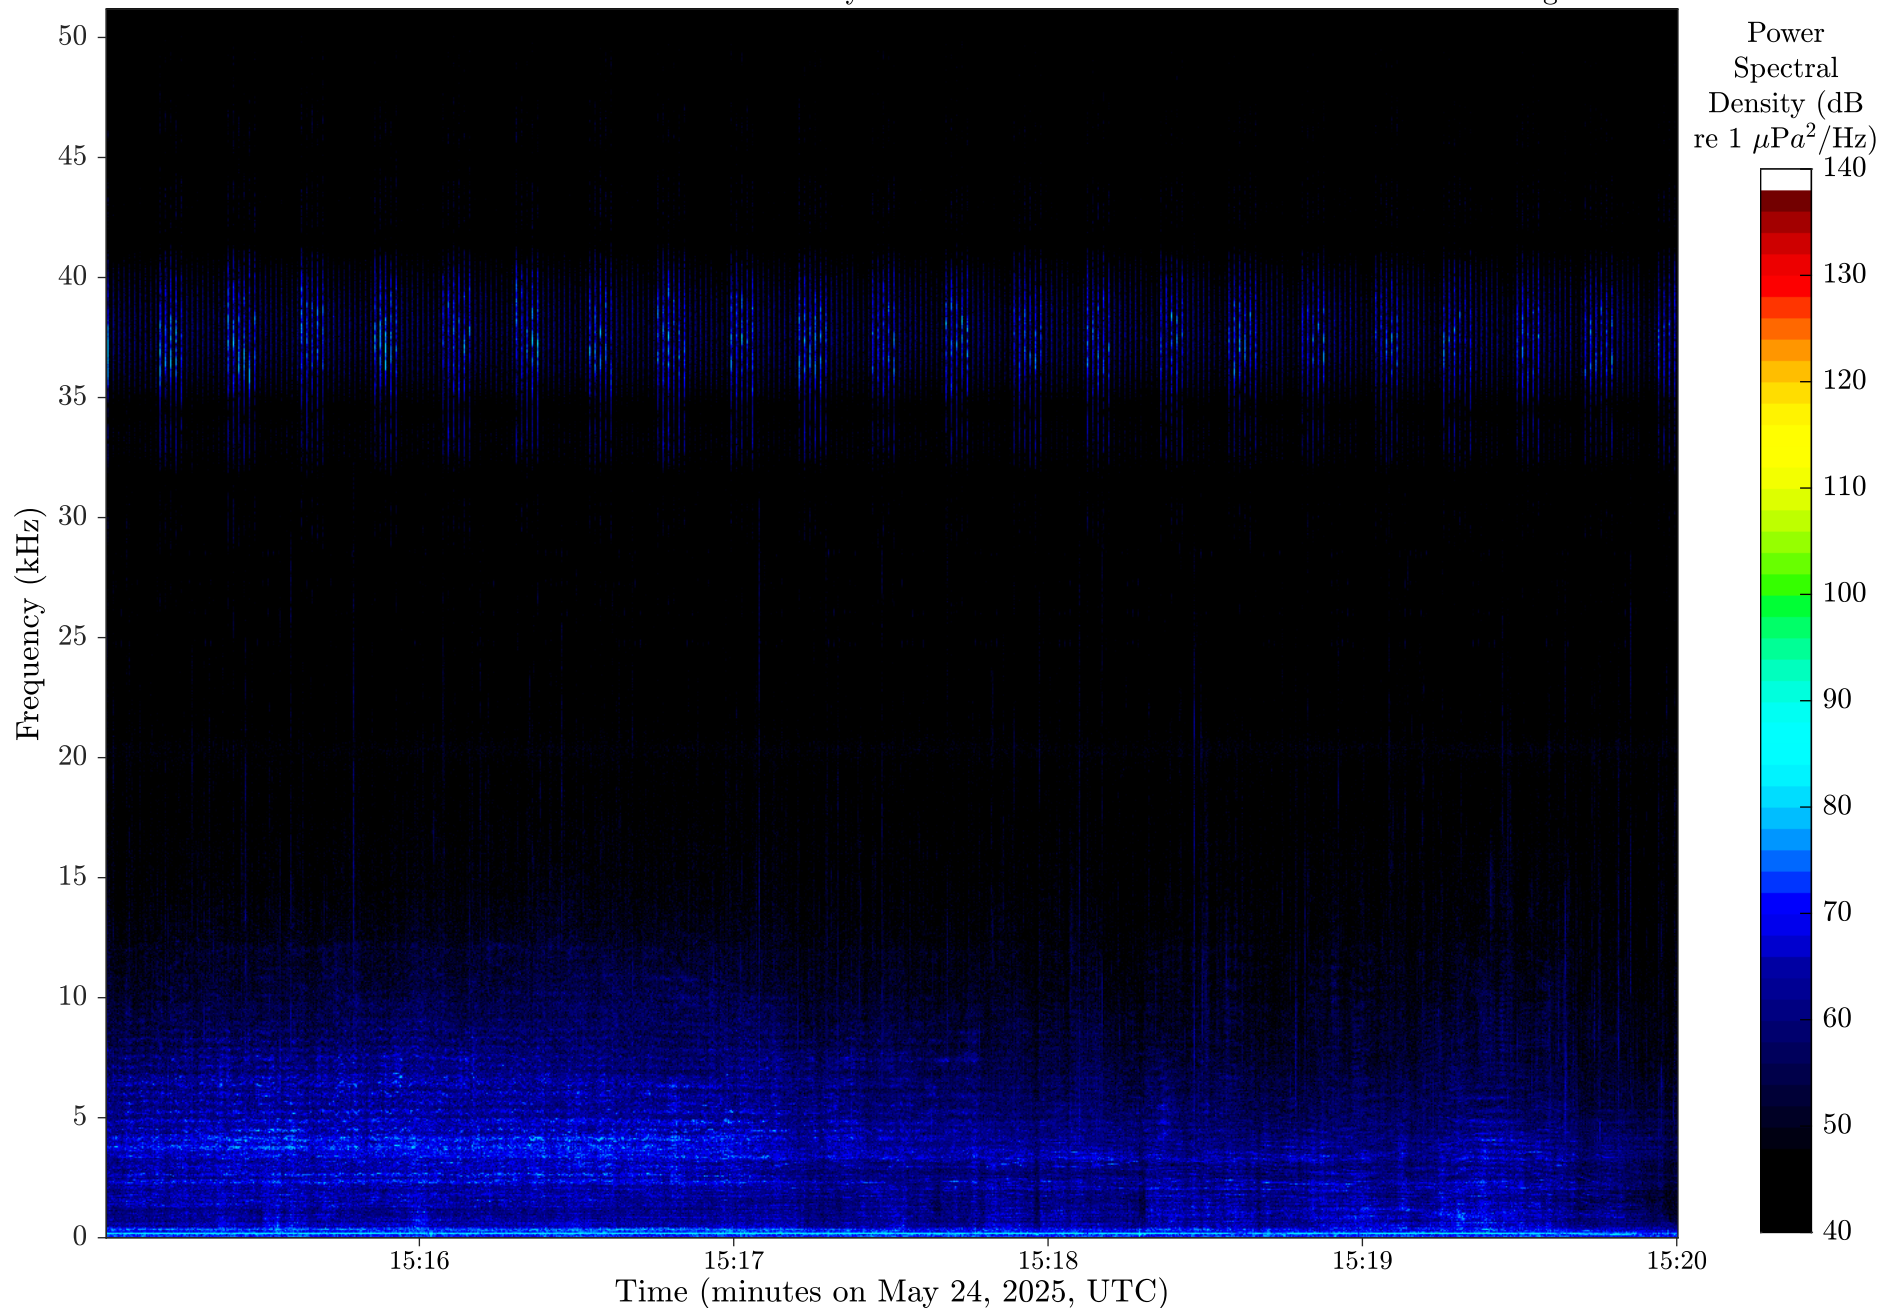


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:27 UTC

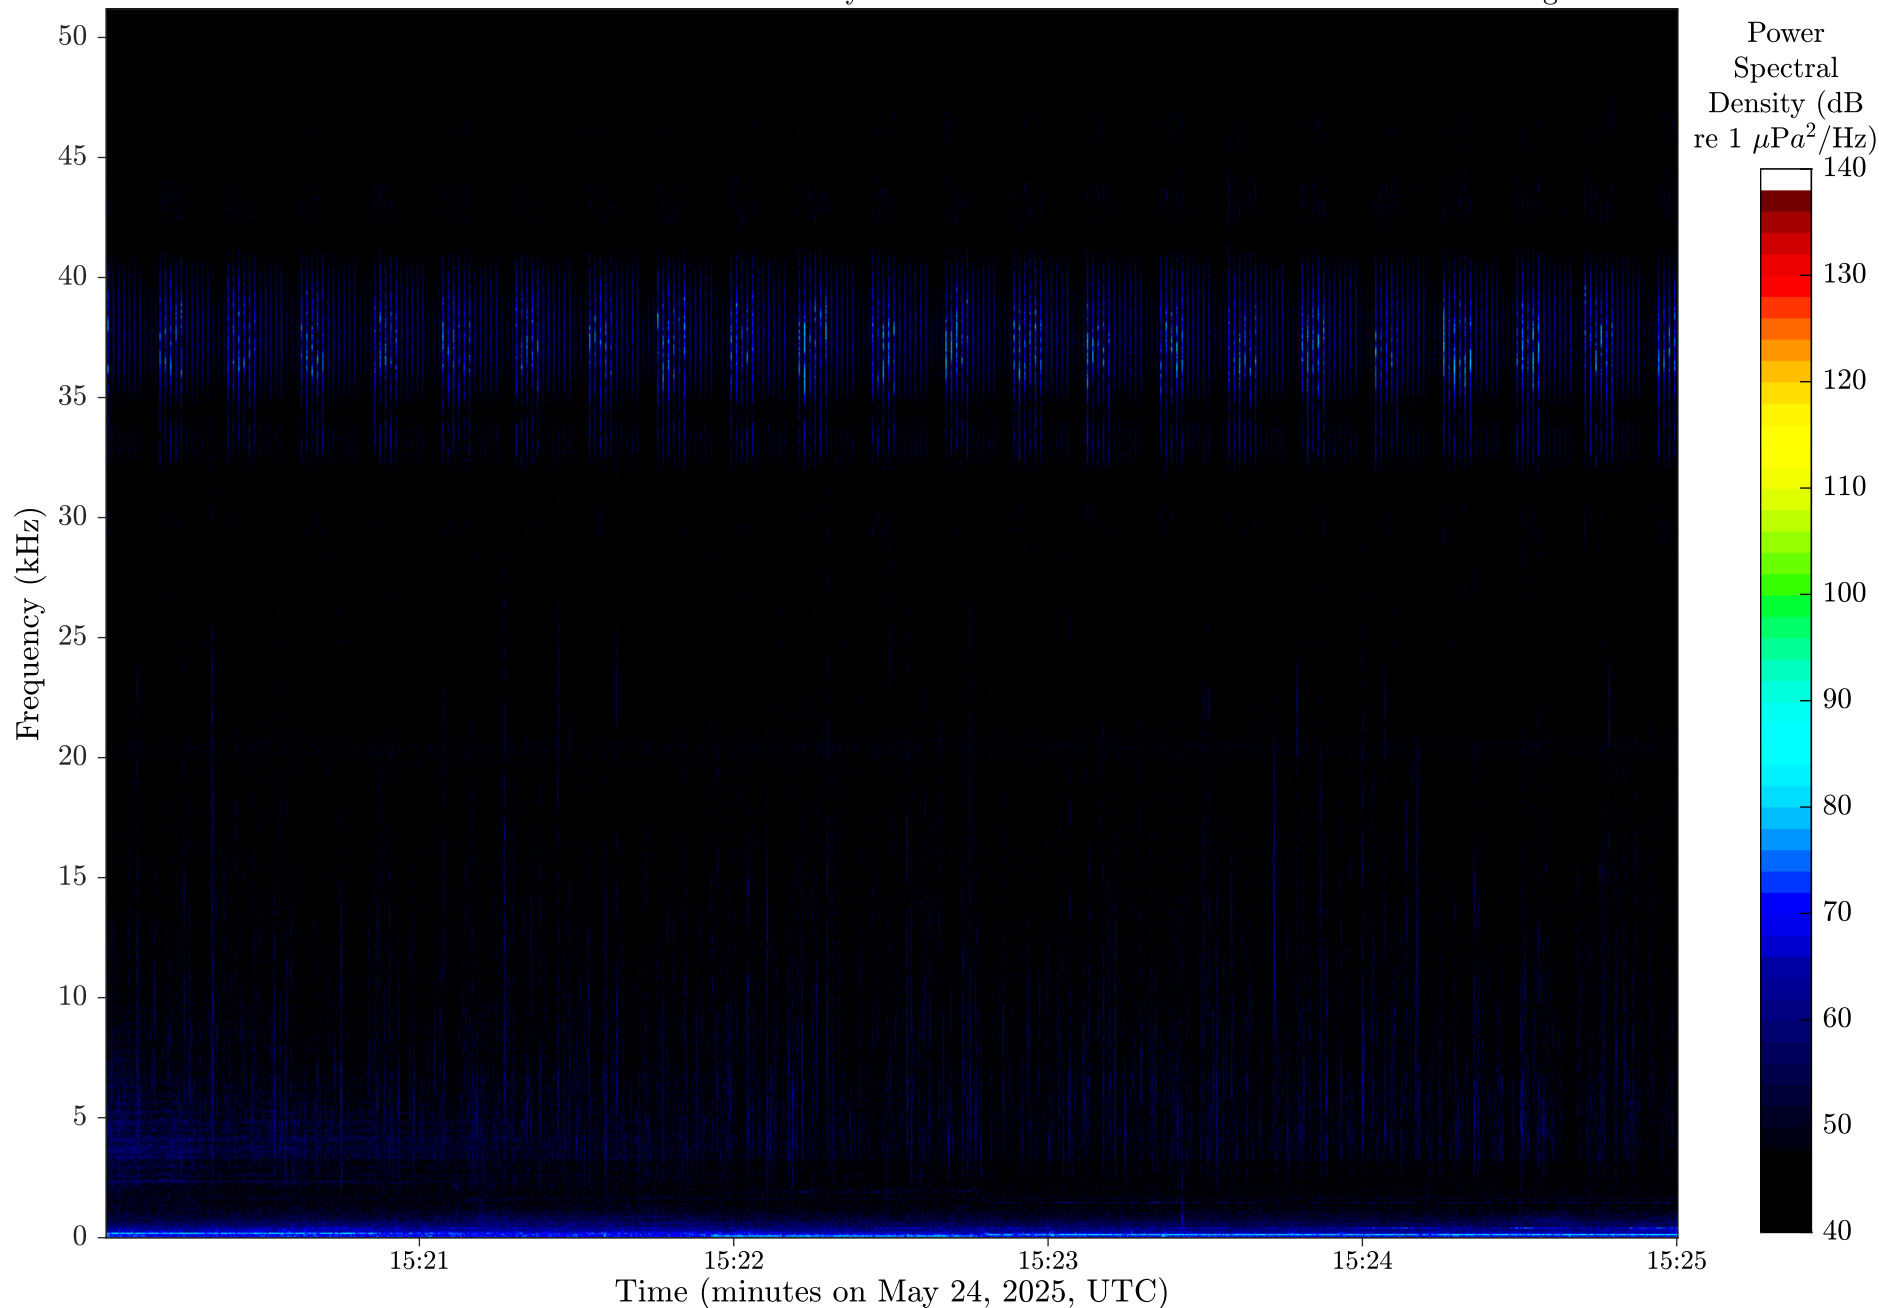


Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:40:36 UTC

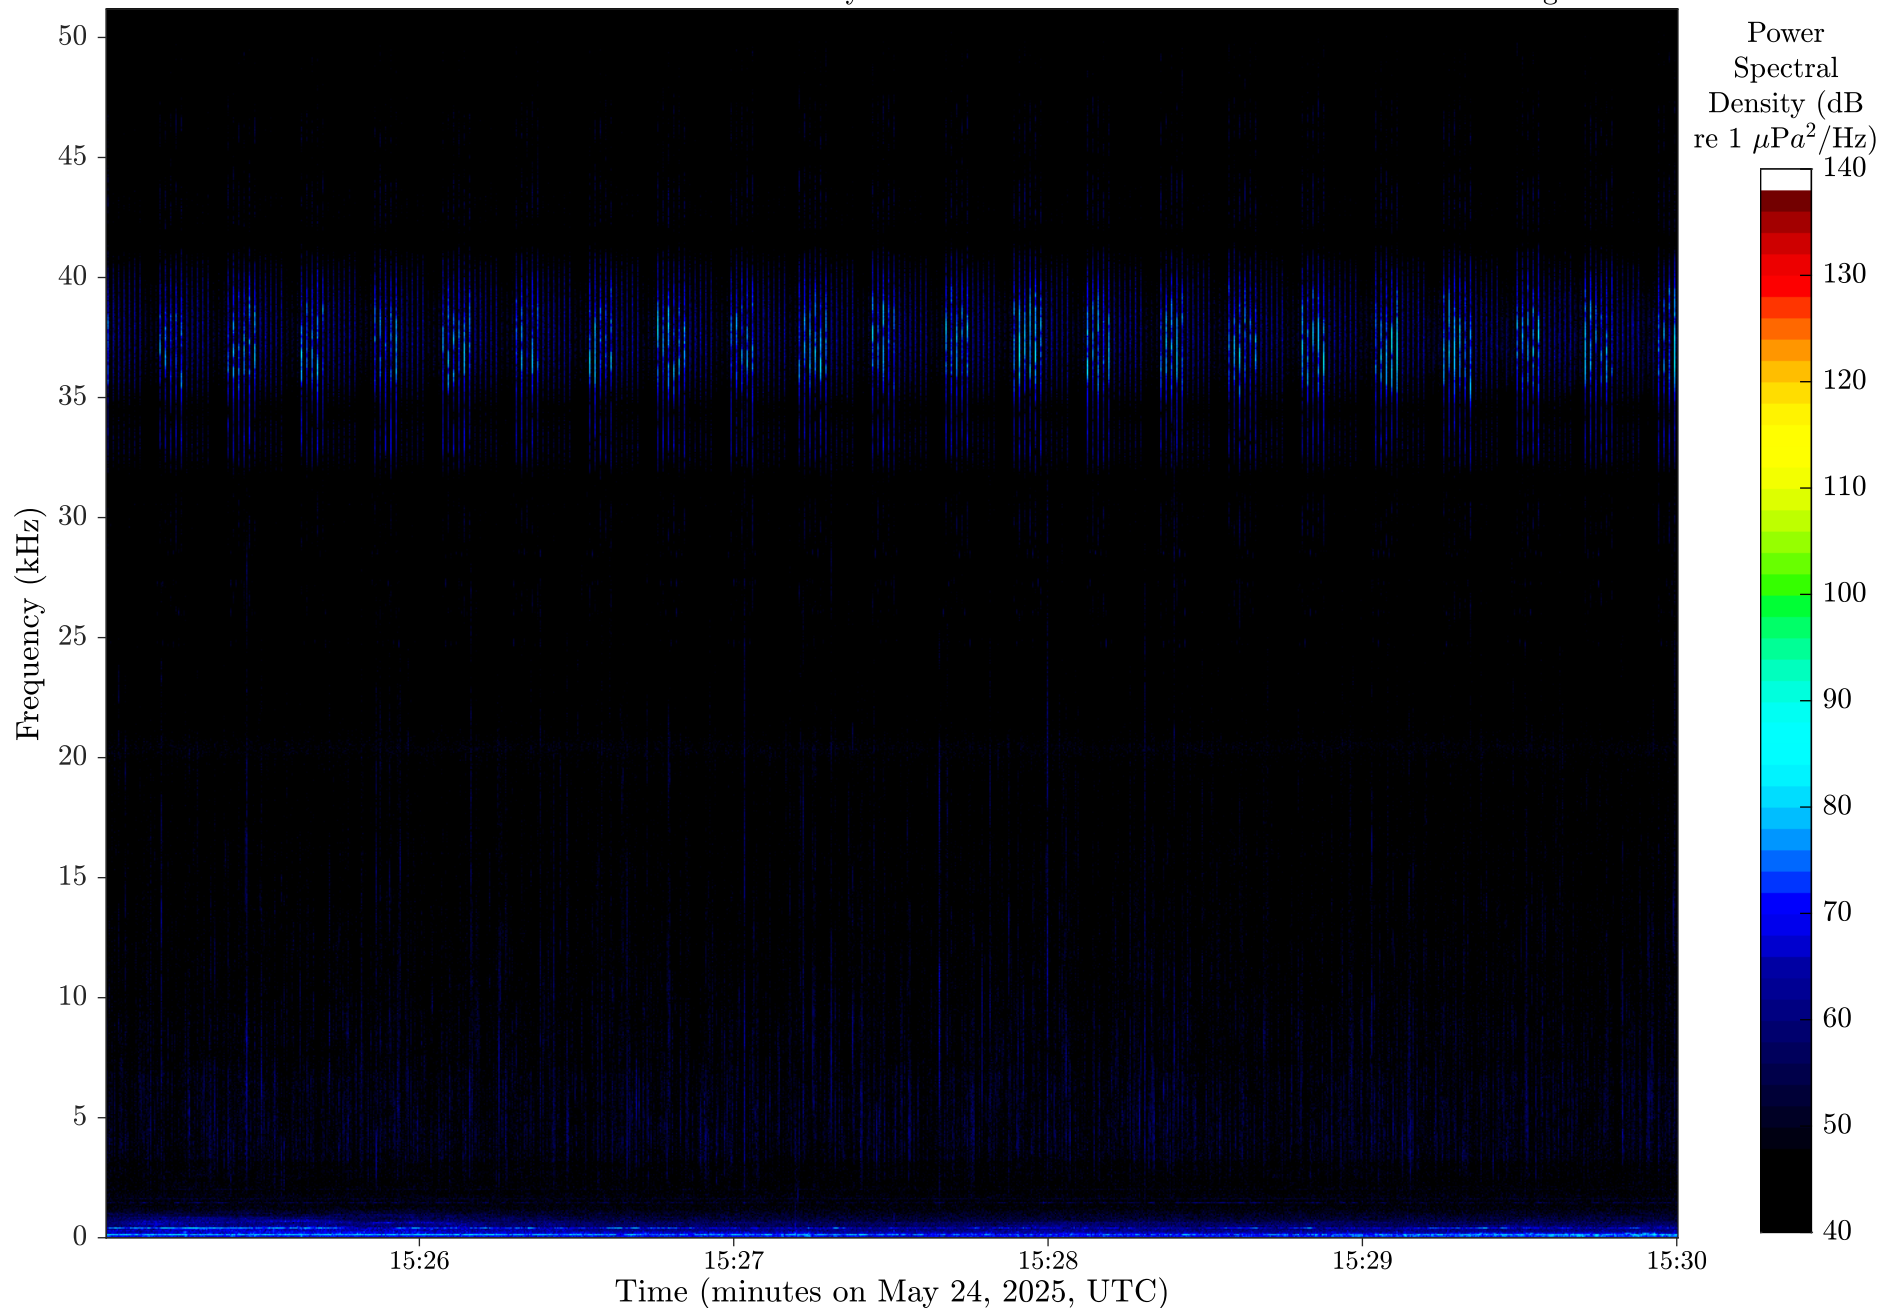

Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:40:43 UTC

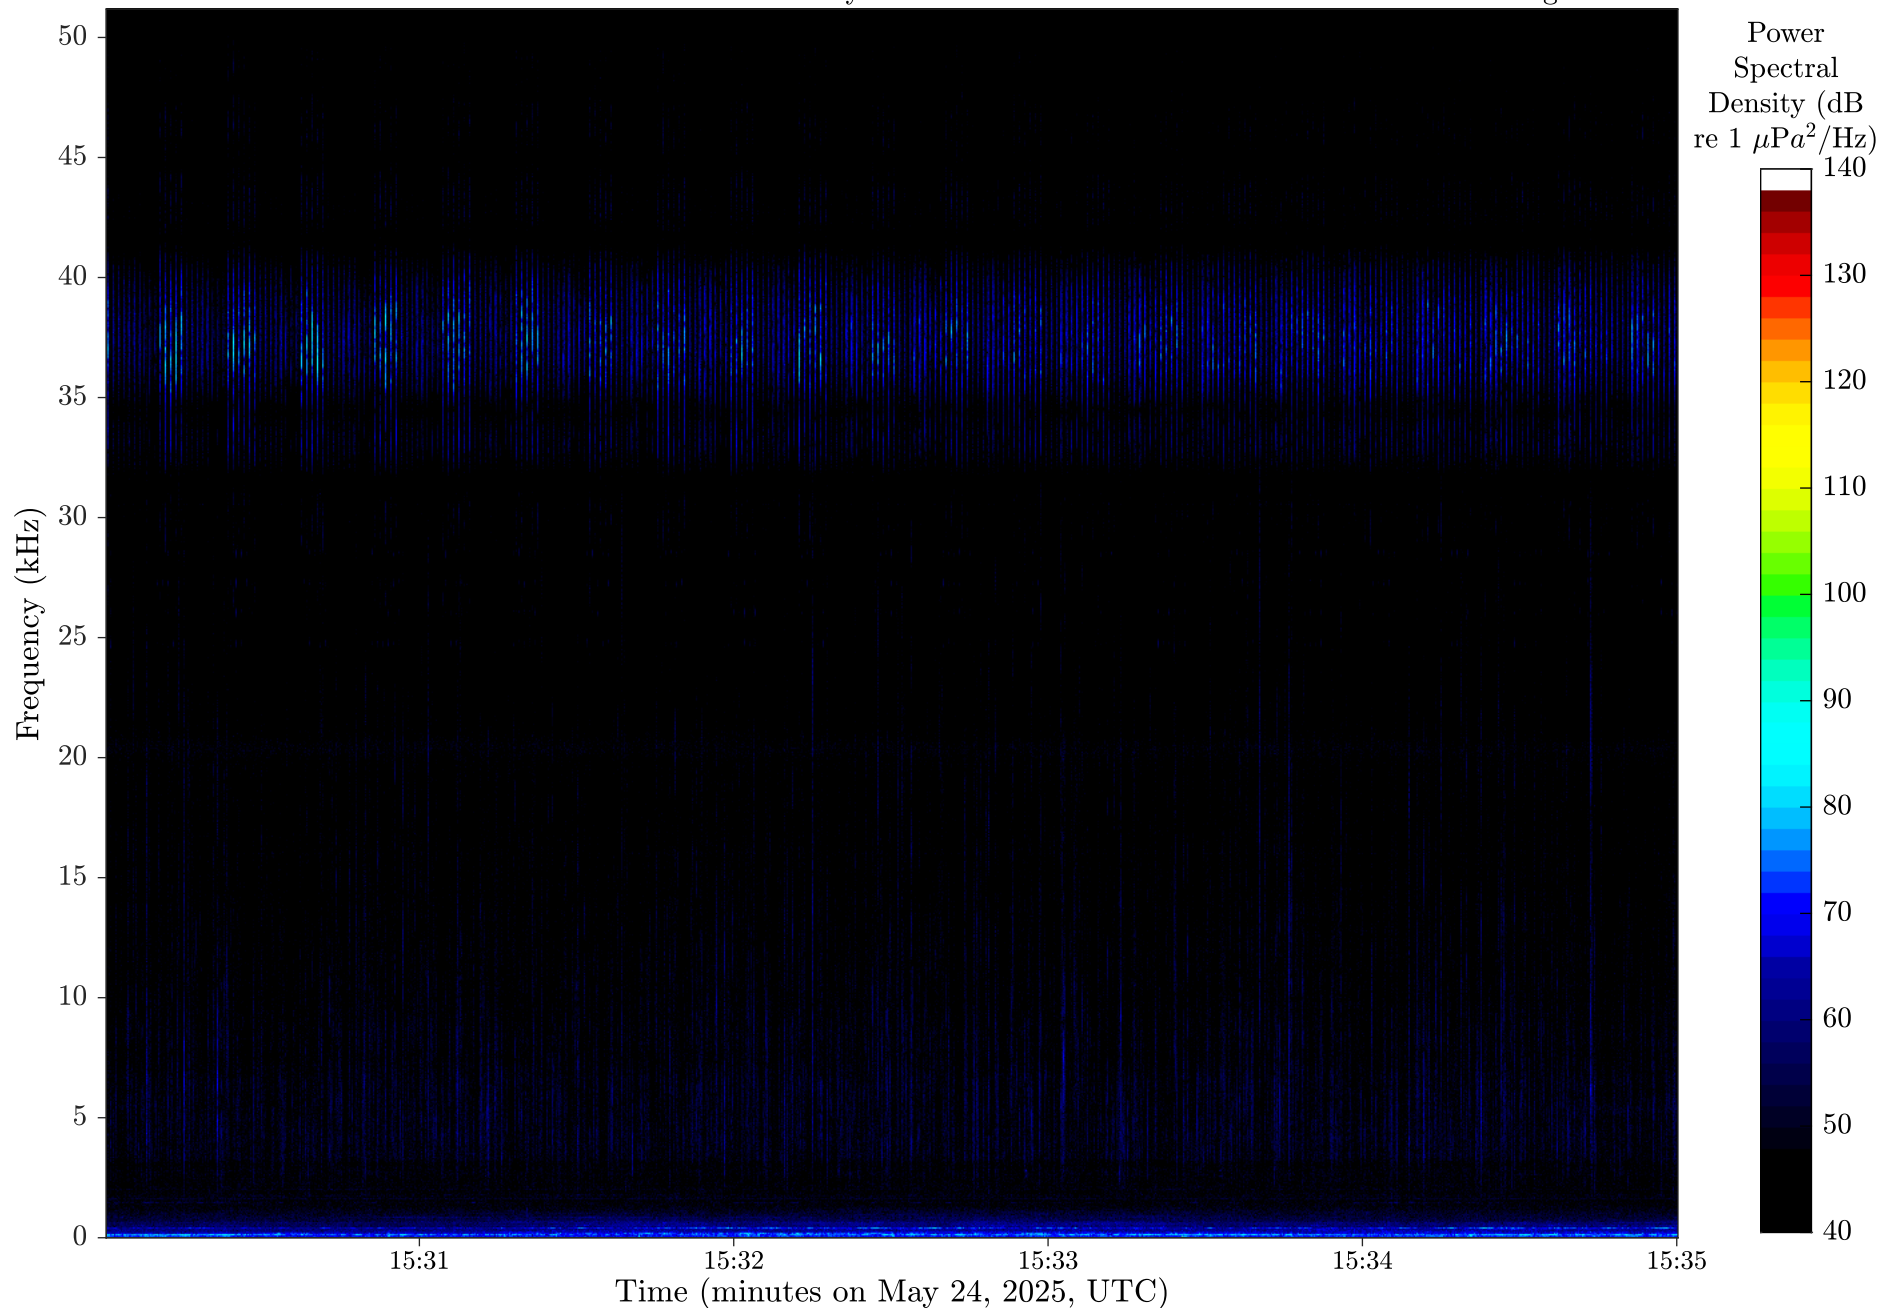

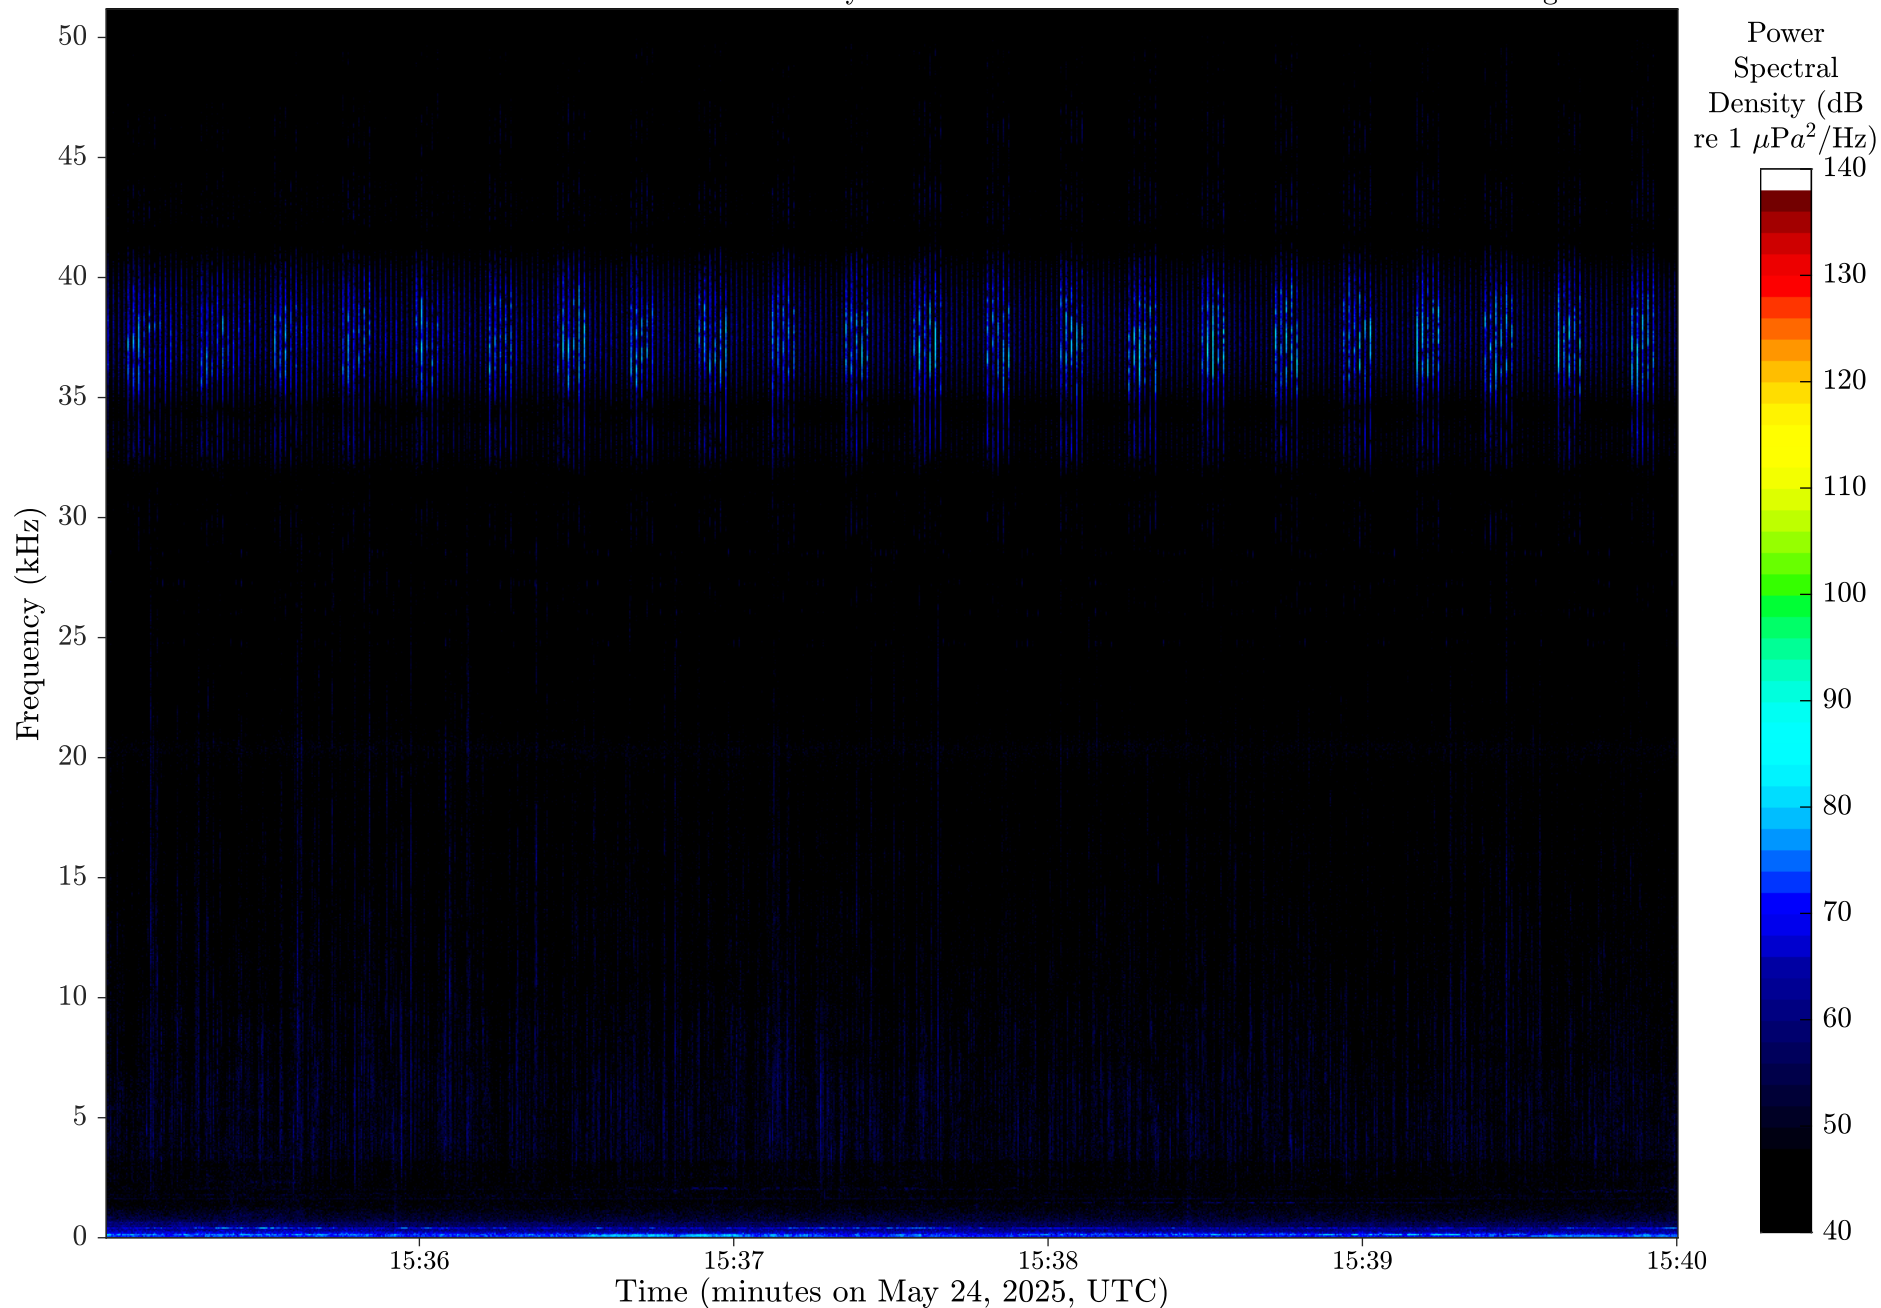


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:00 UTC

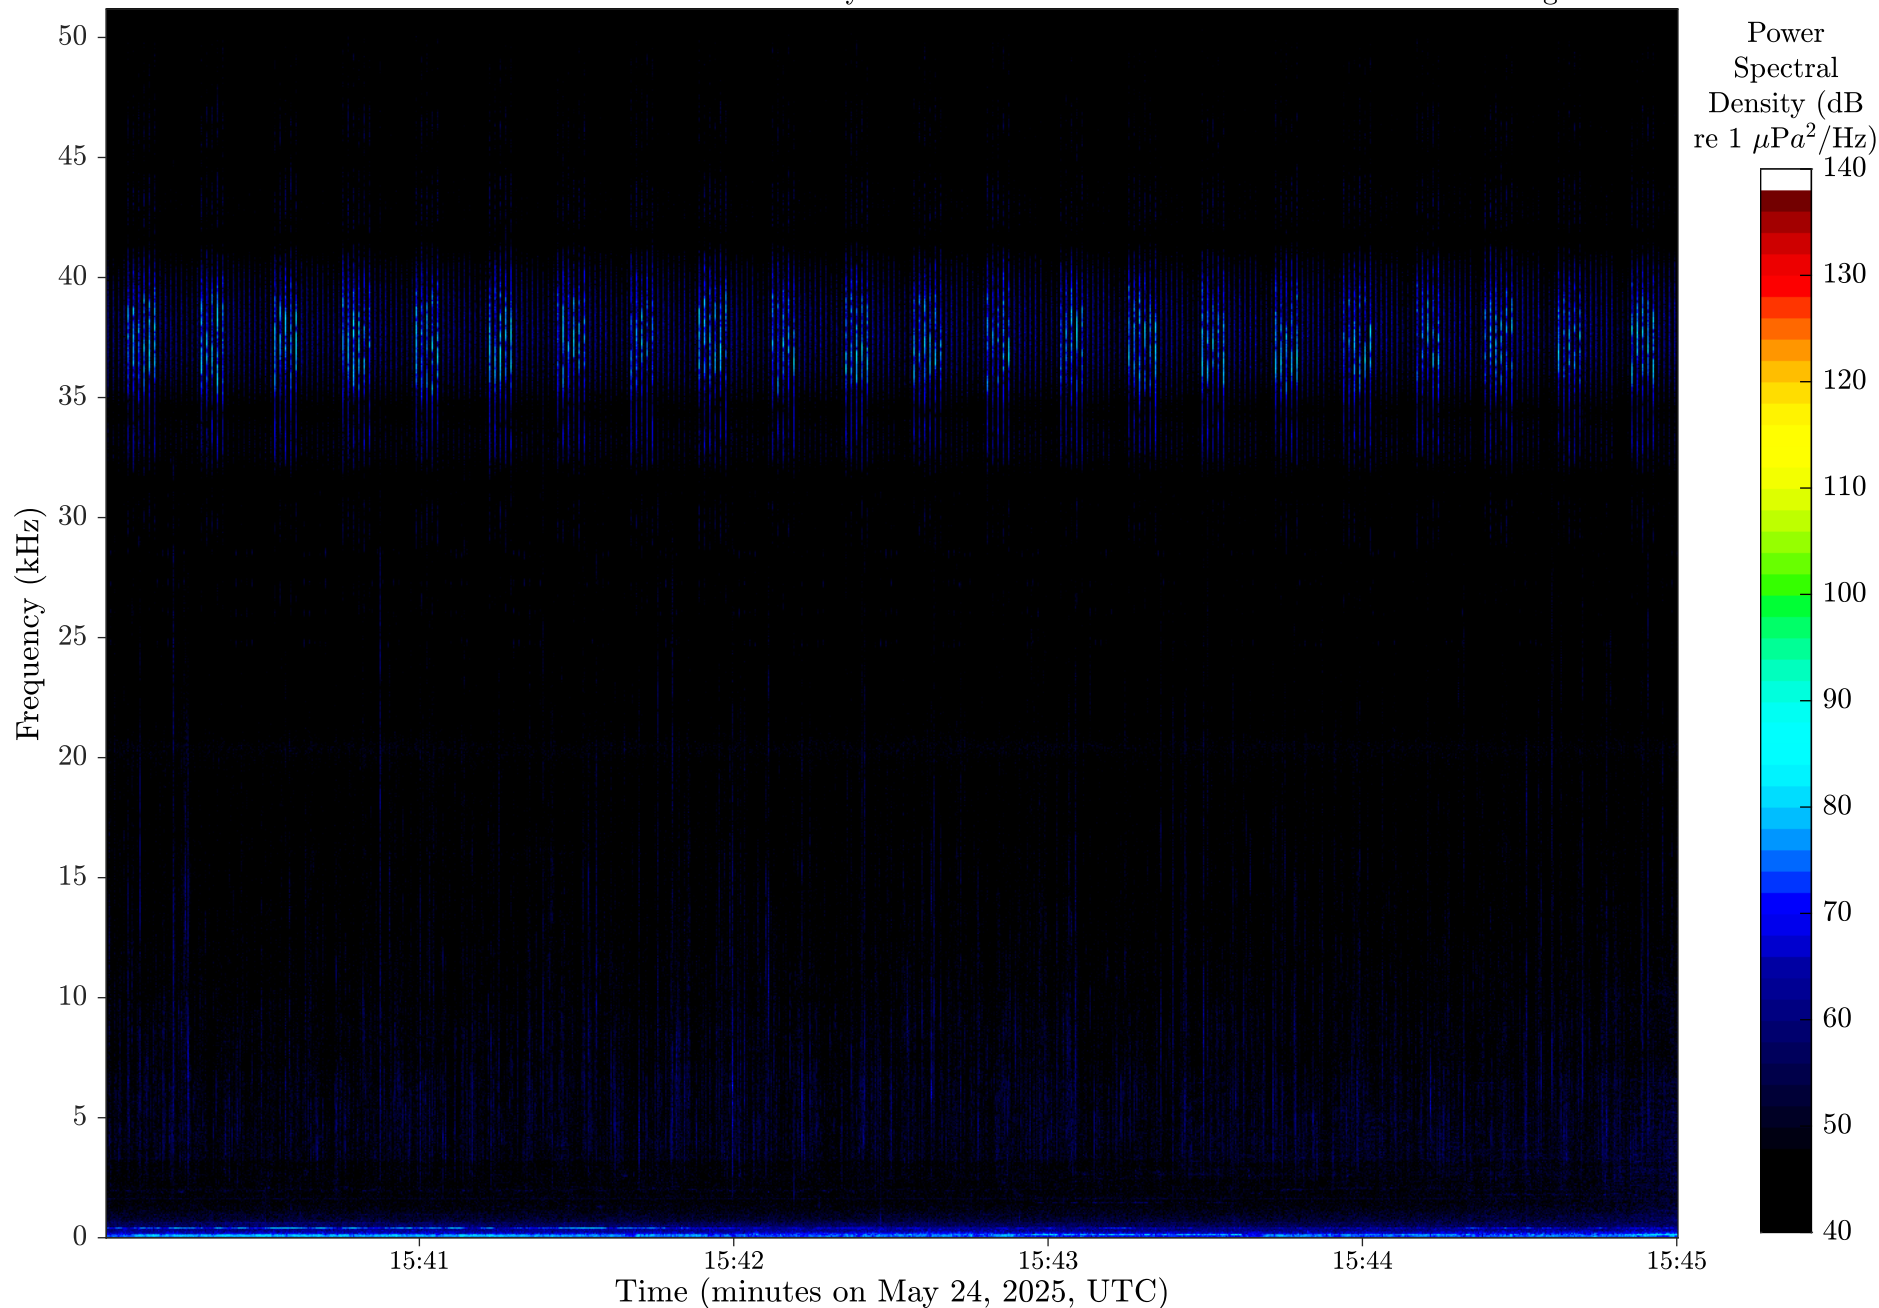


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:08 UTC

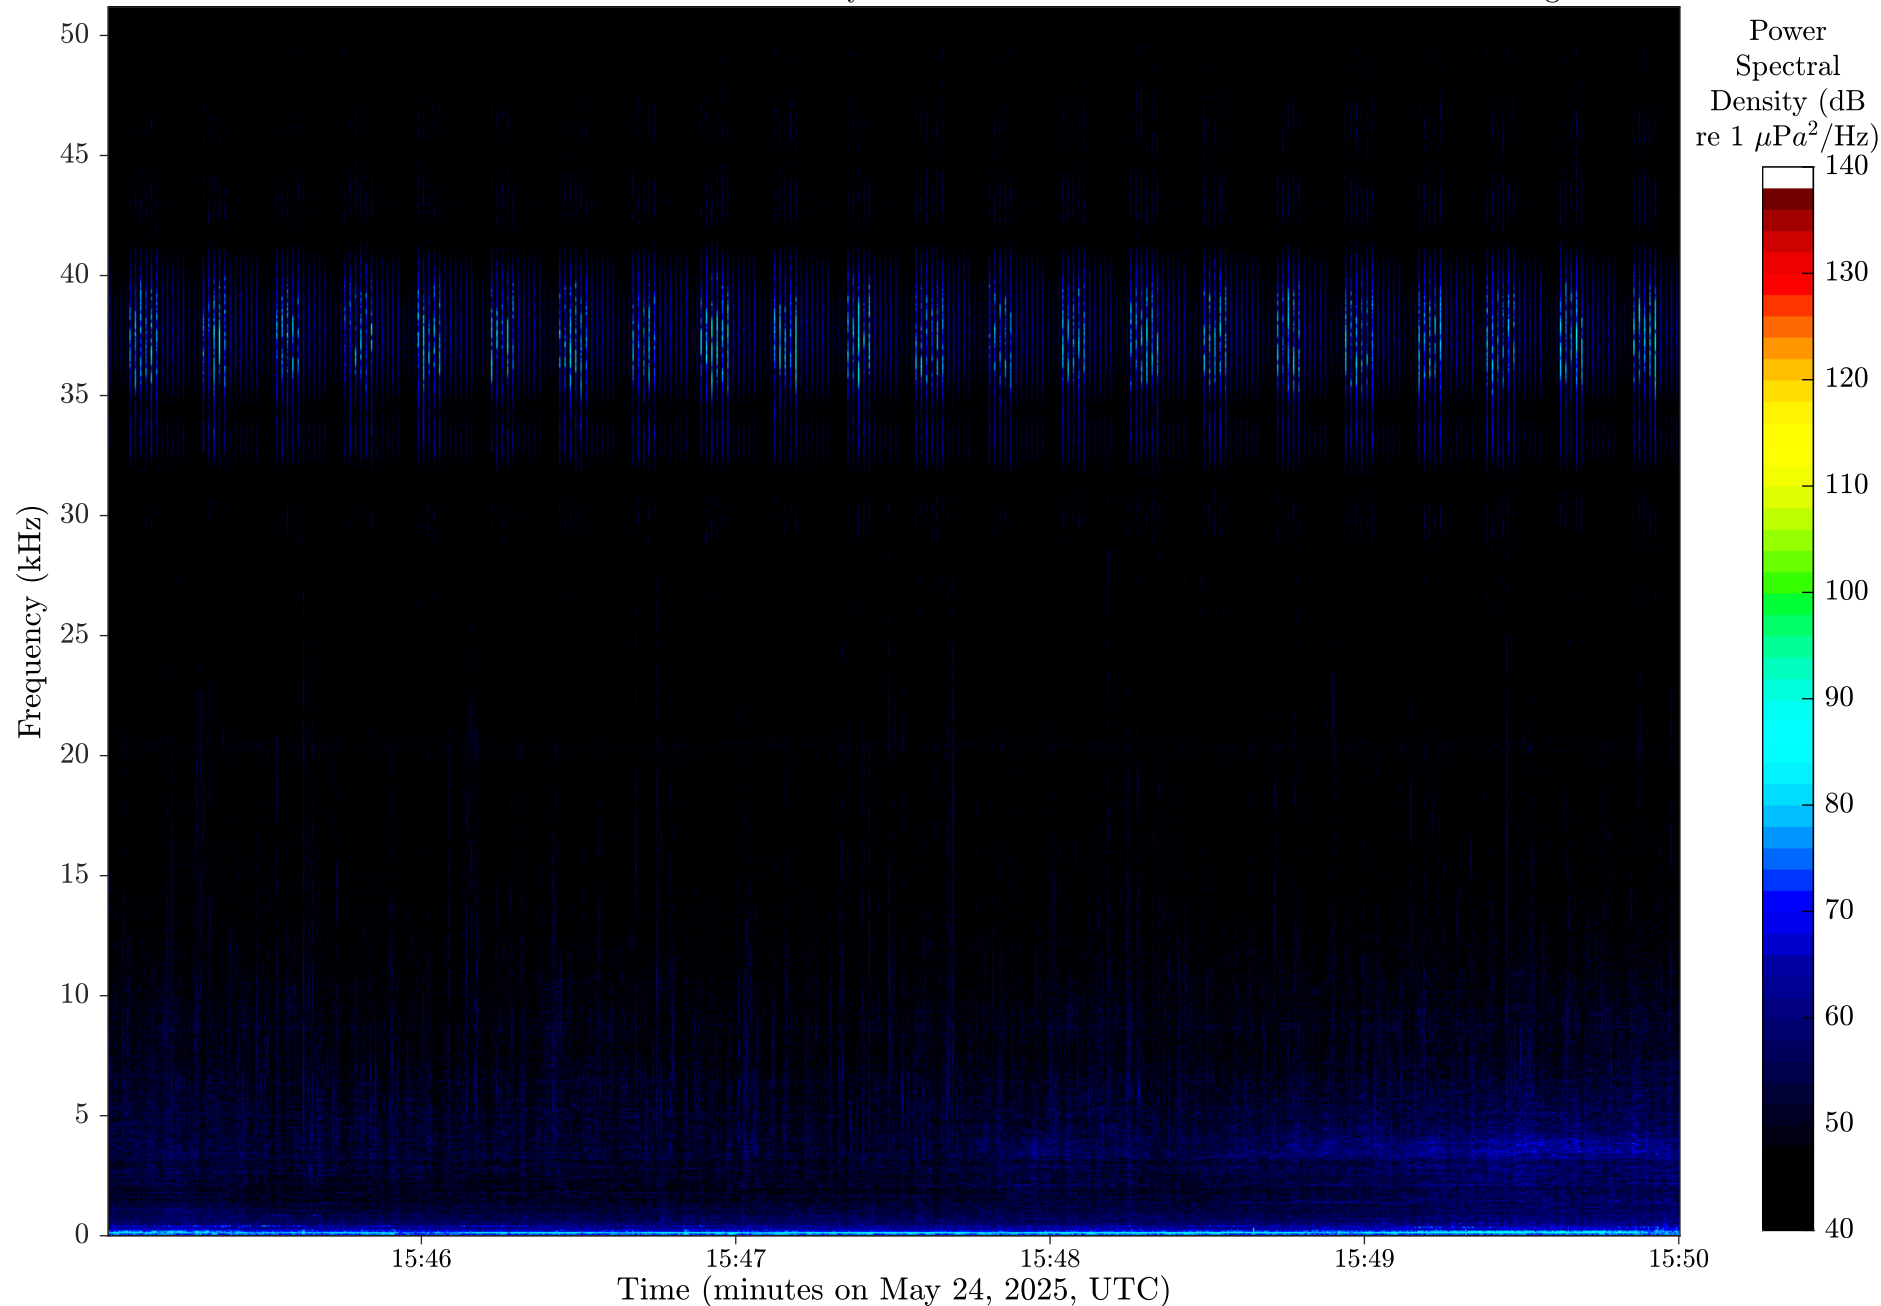


Comments: 32.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:16 UTC

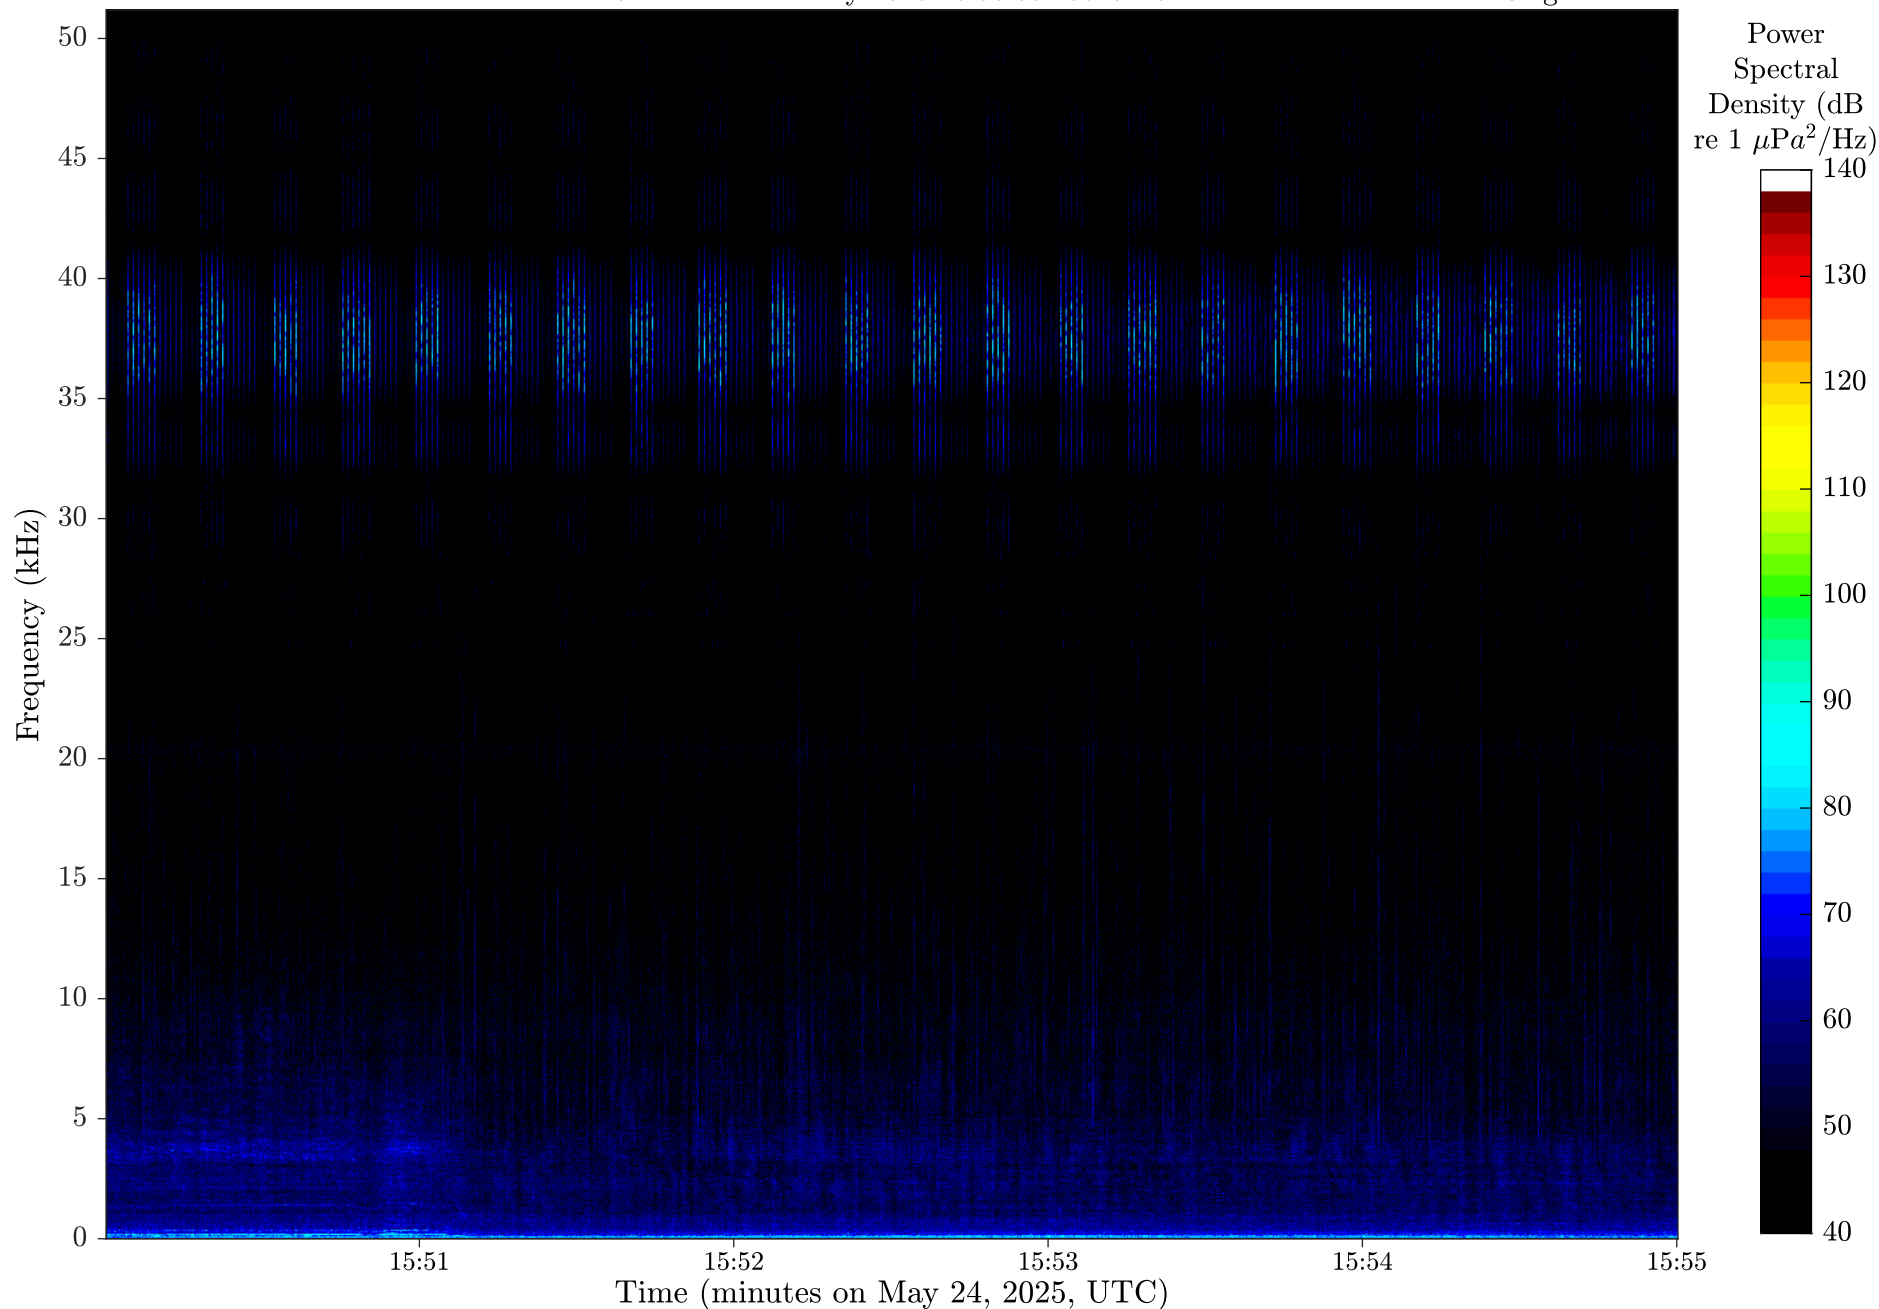


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:24 UTC

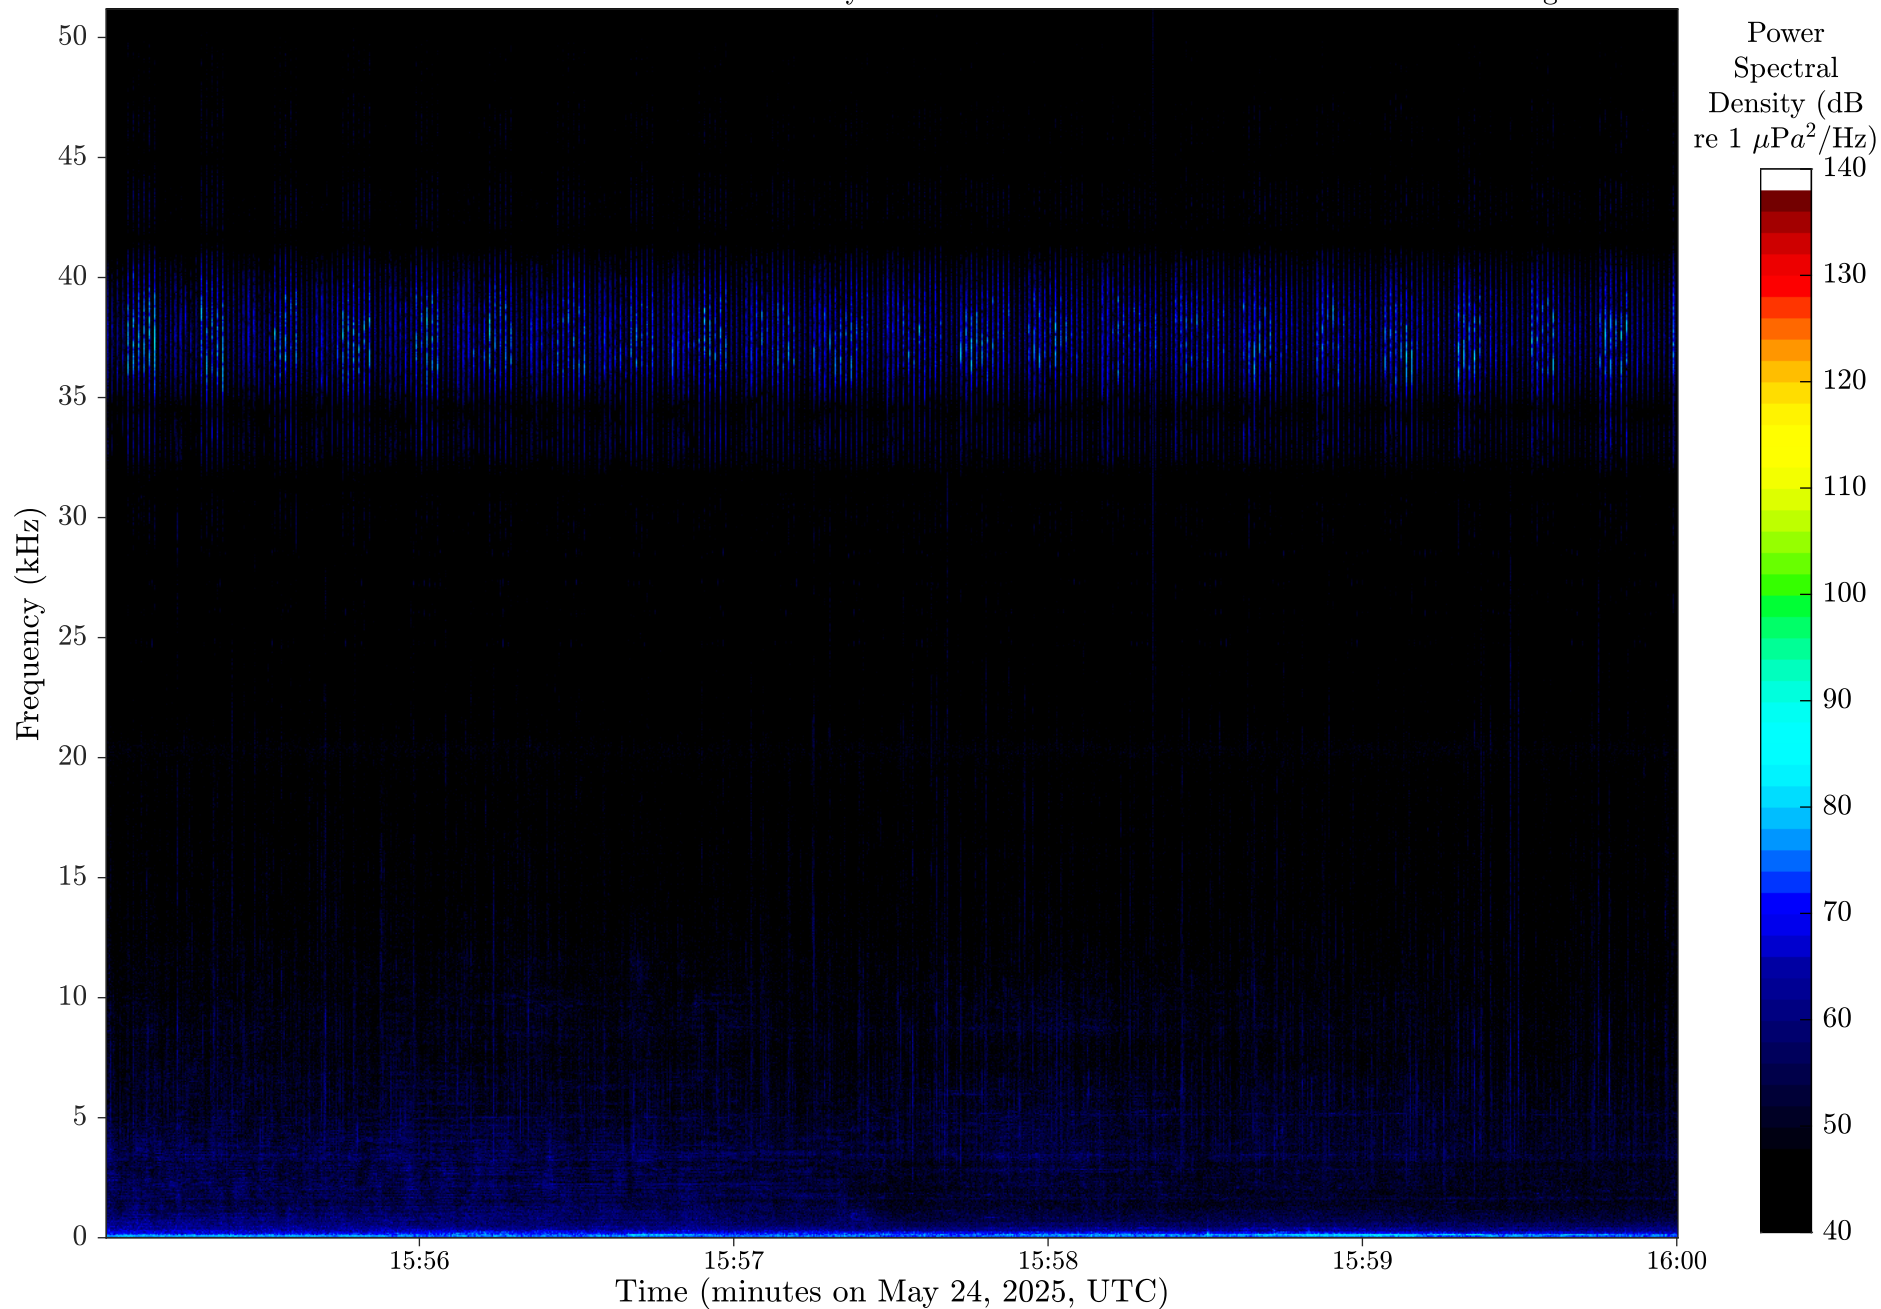


Comments: 31 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:33 UTC

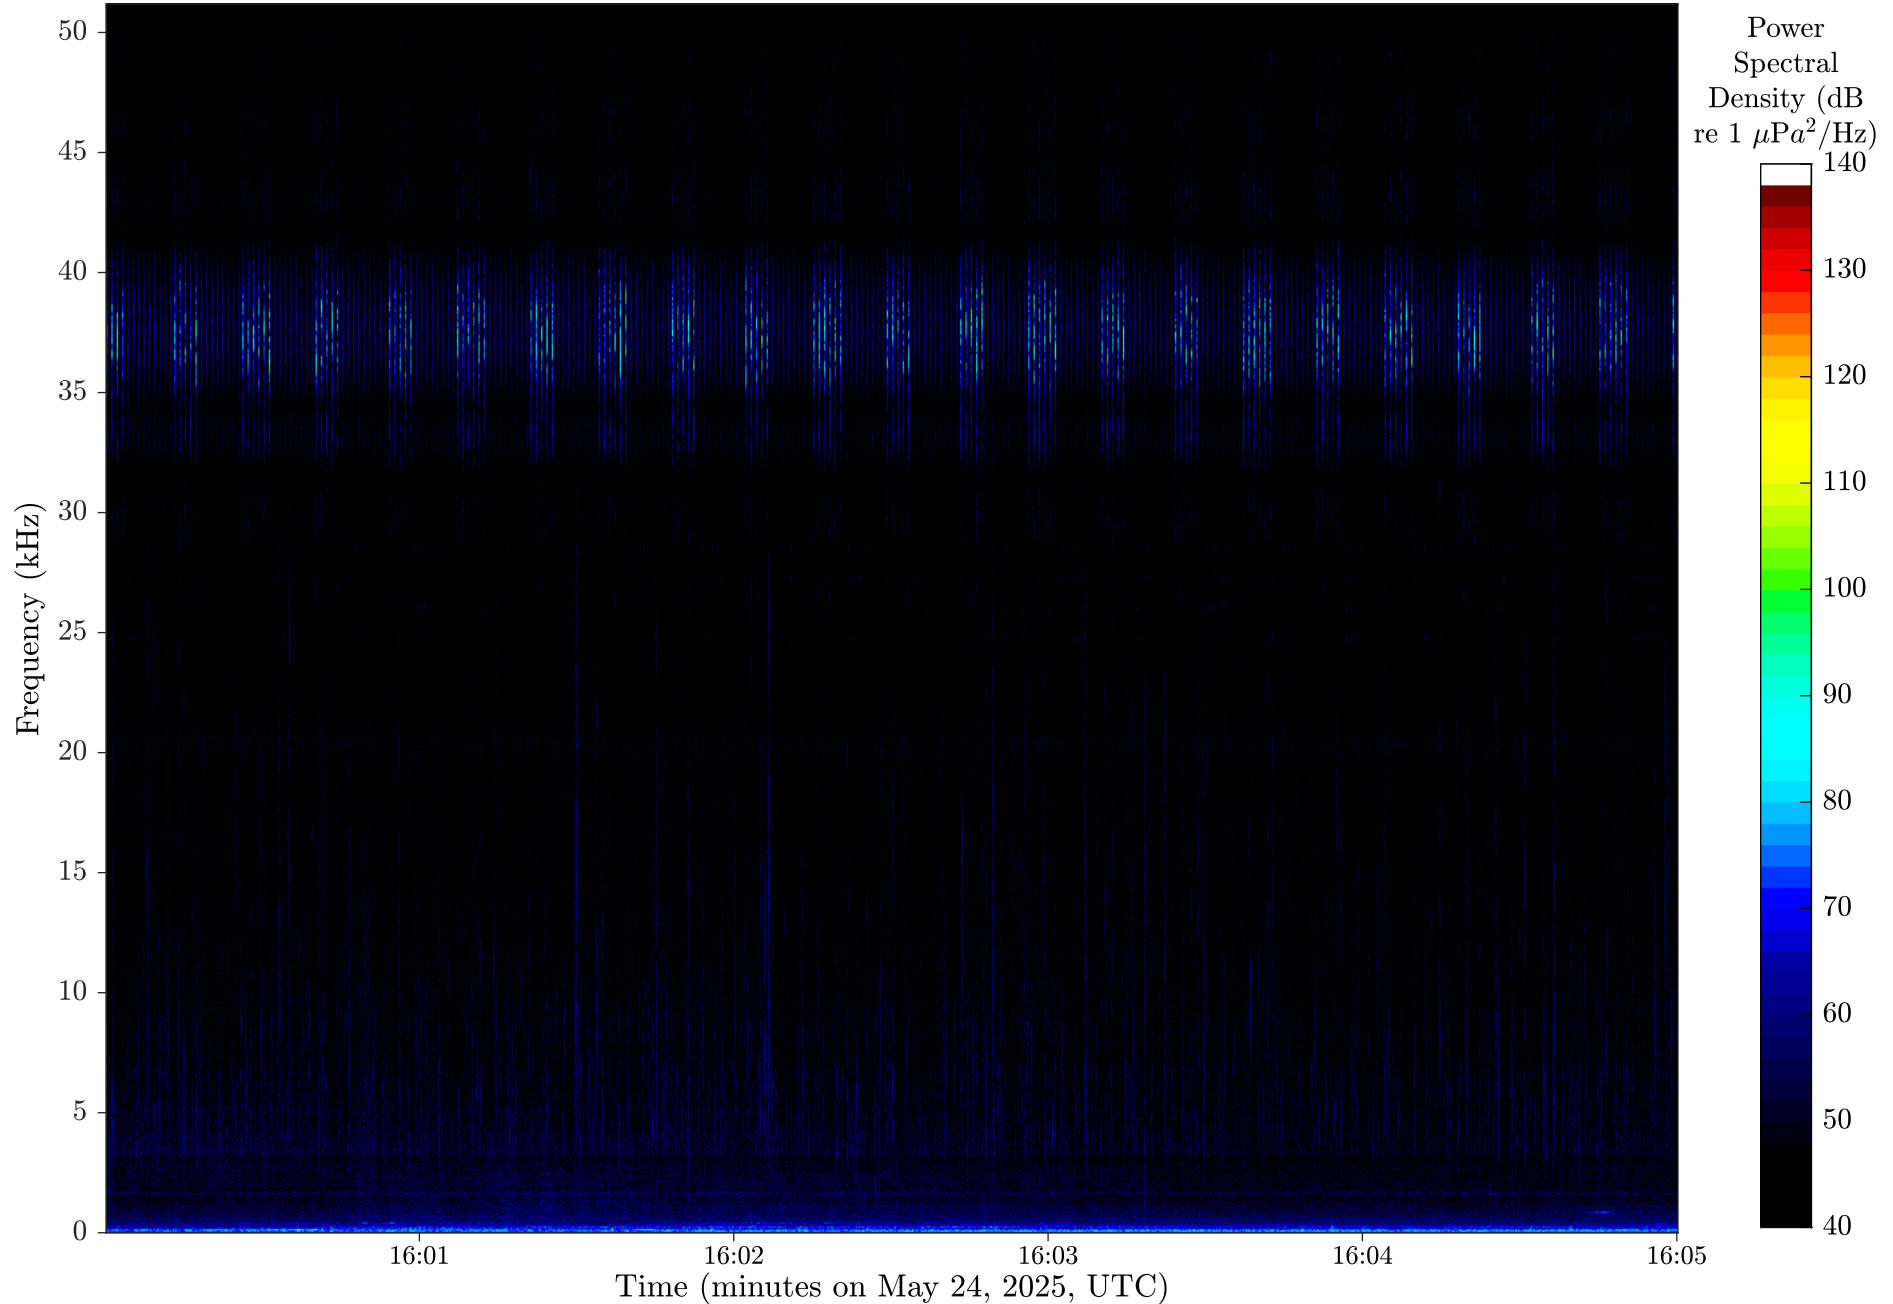


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:41 UTC

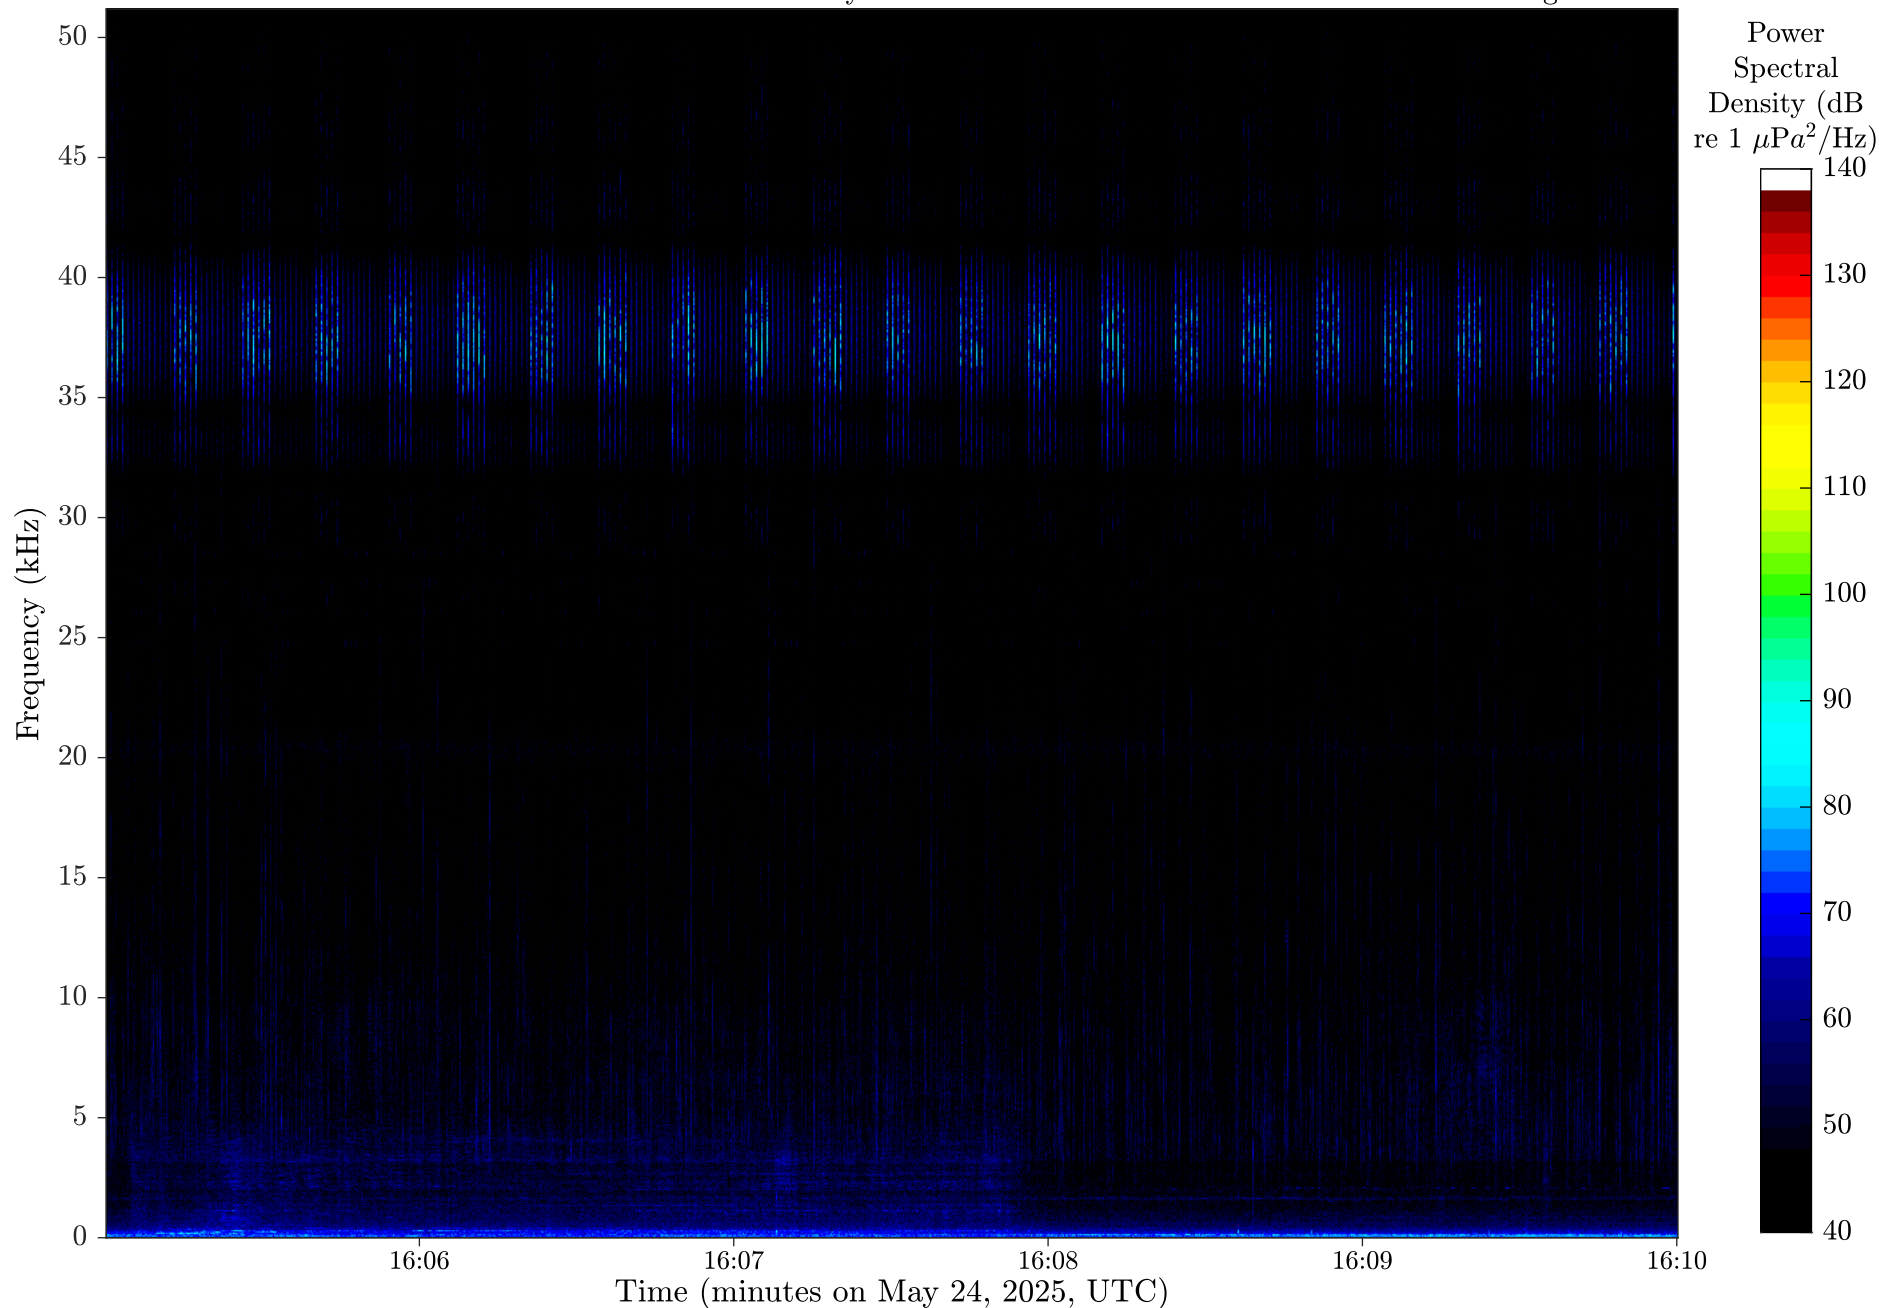


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:41:49 UTC

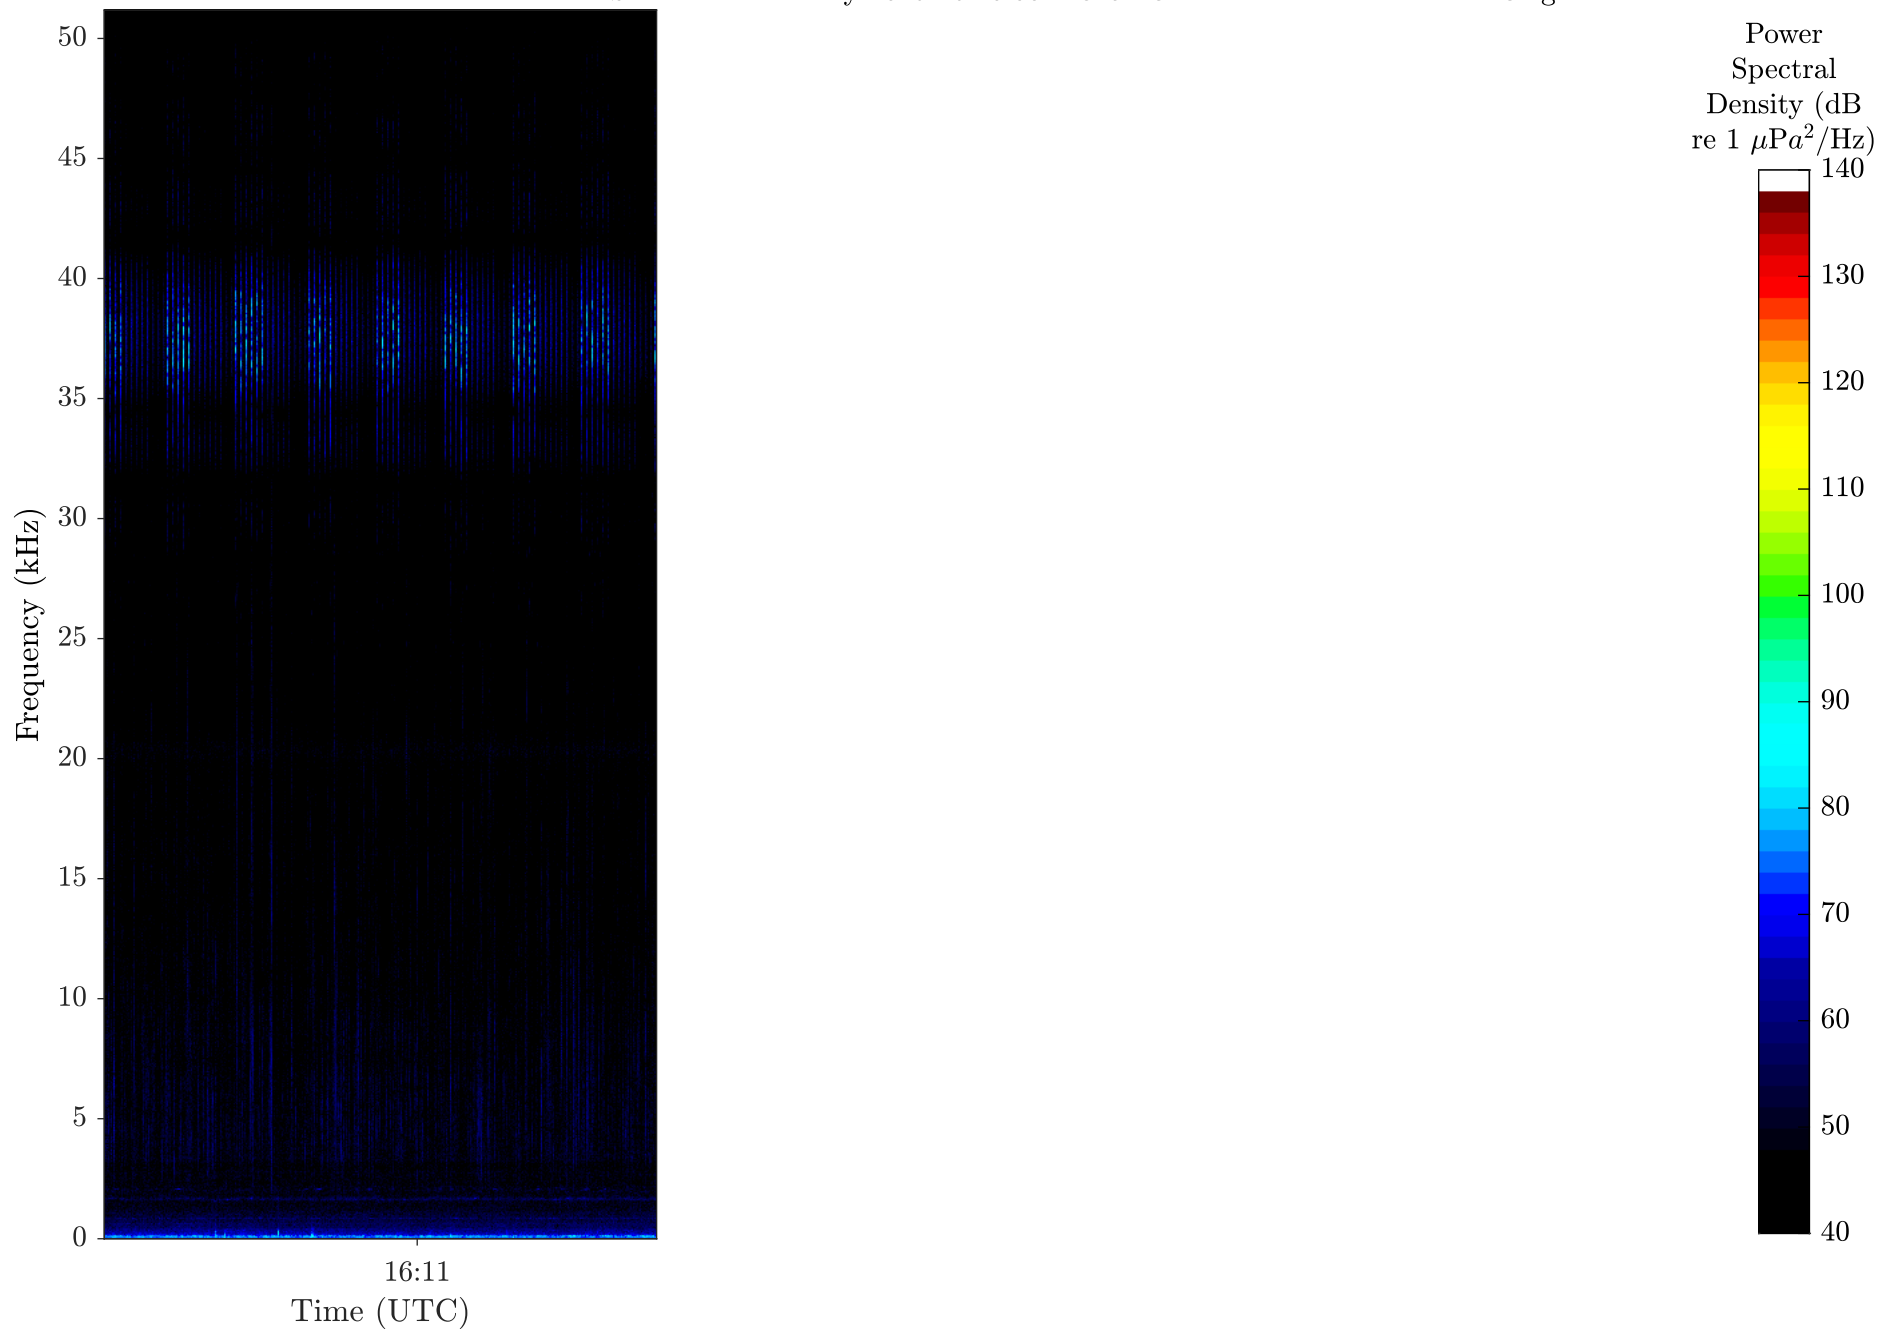

Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:41:53 UTC

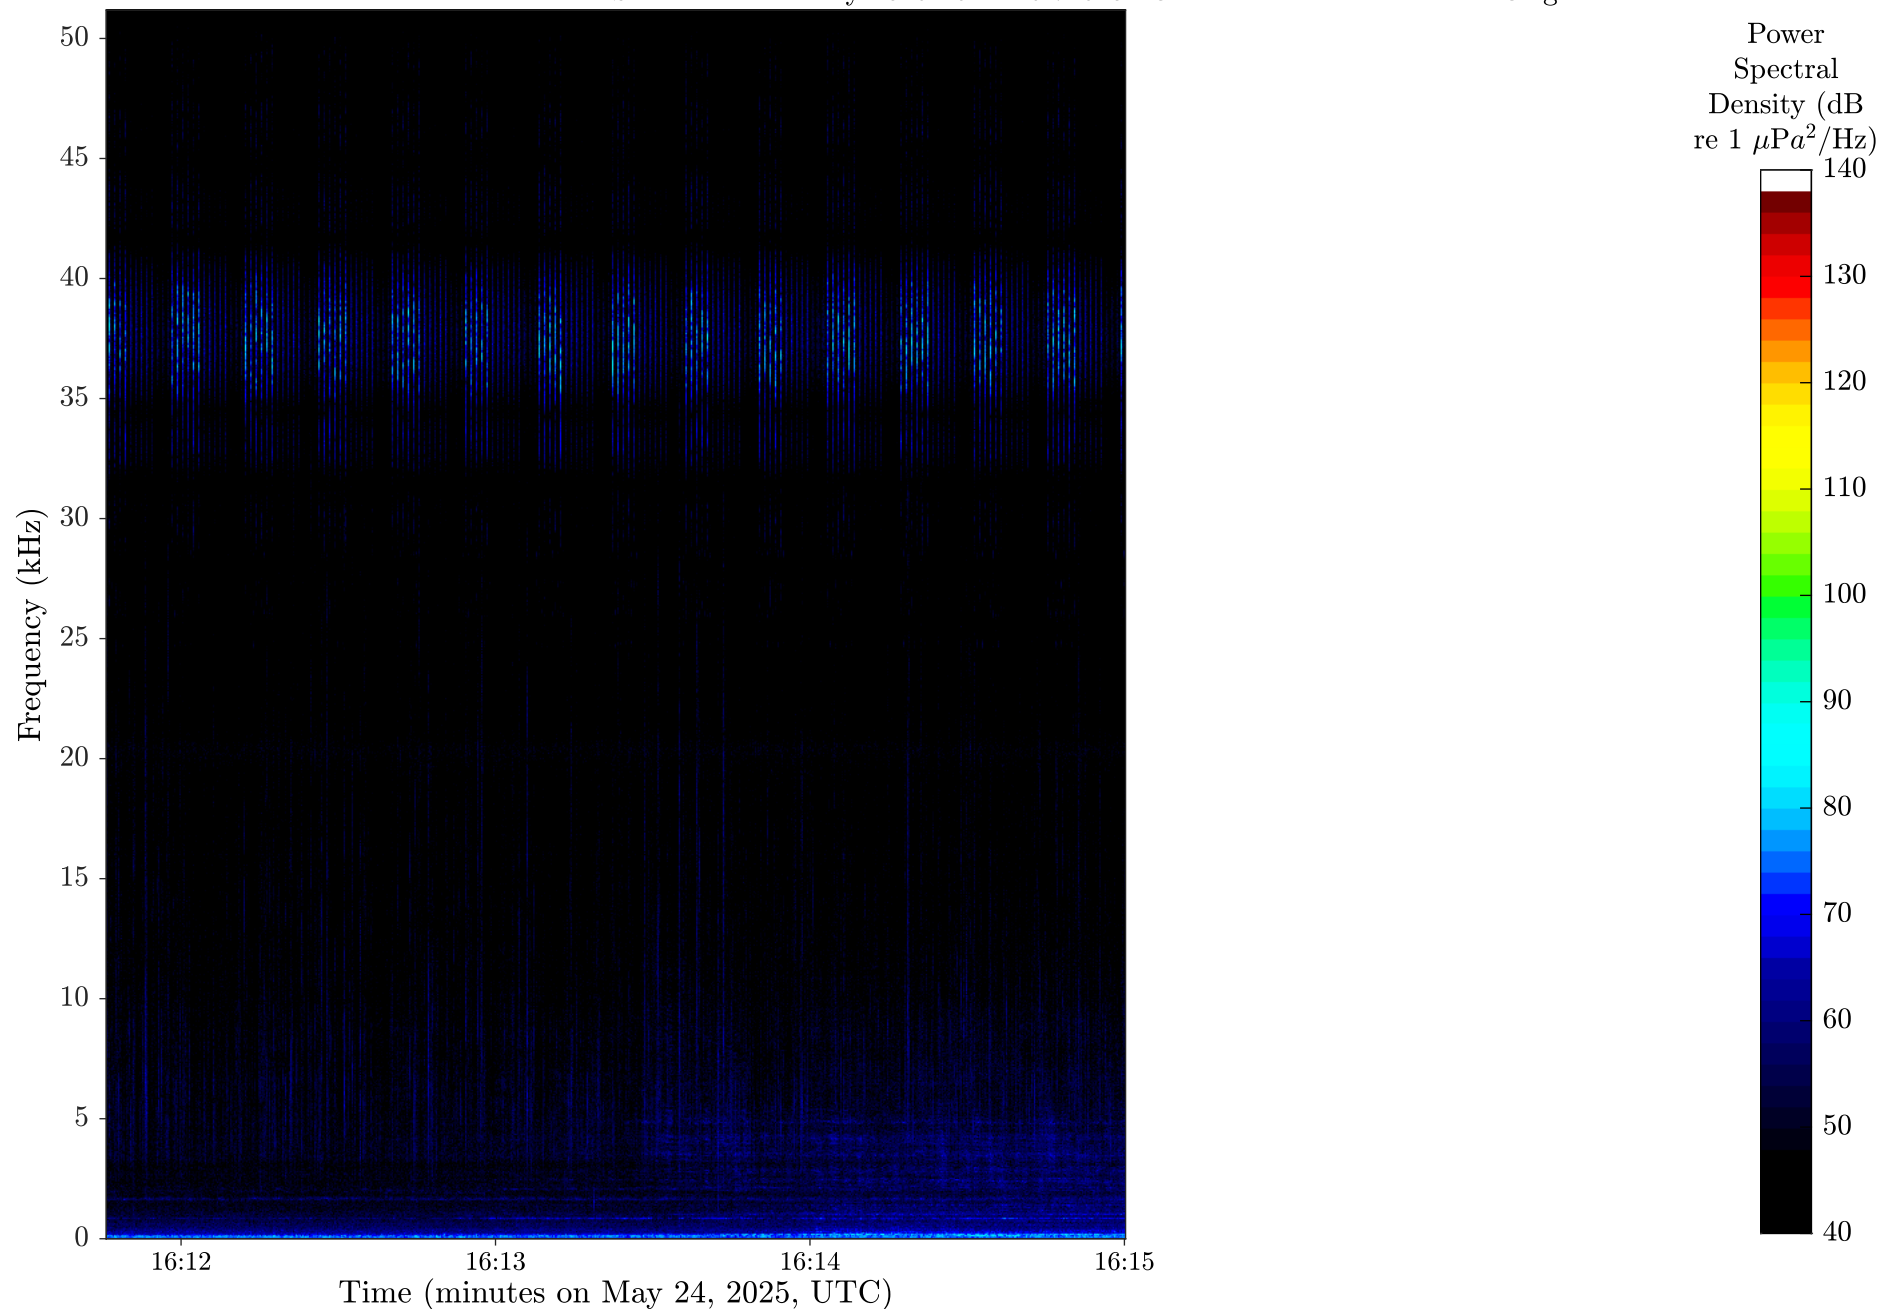

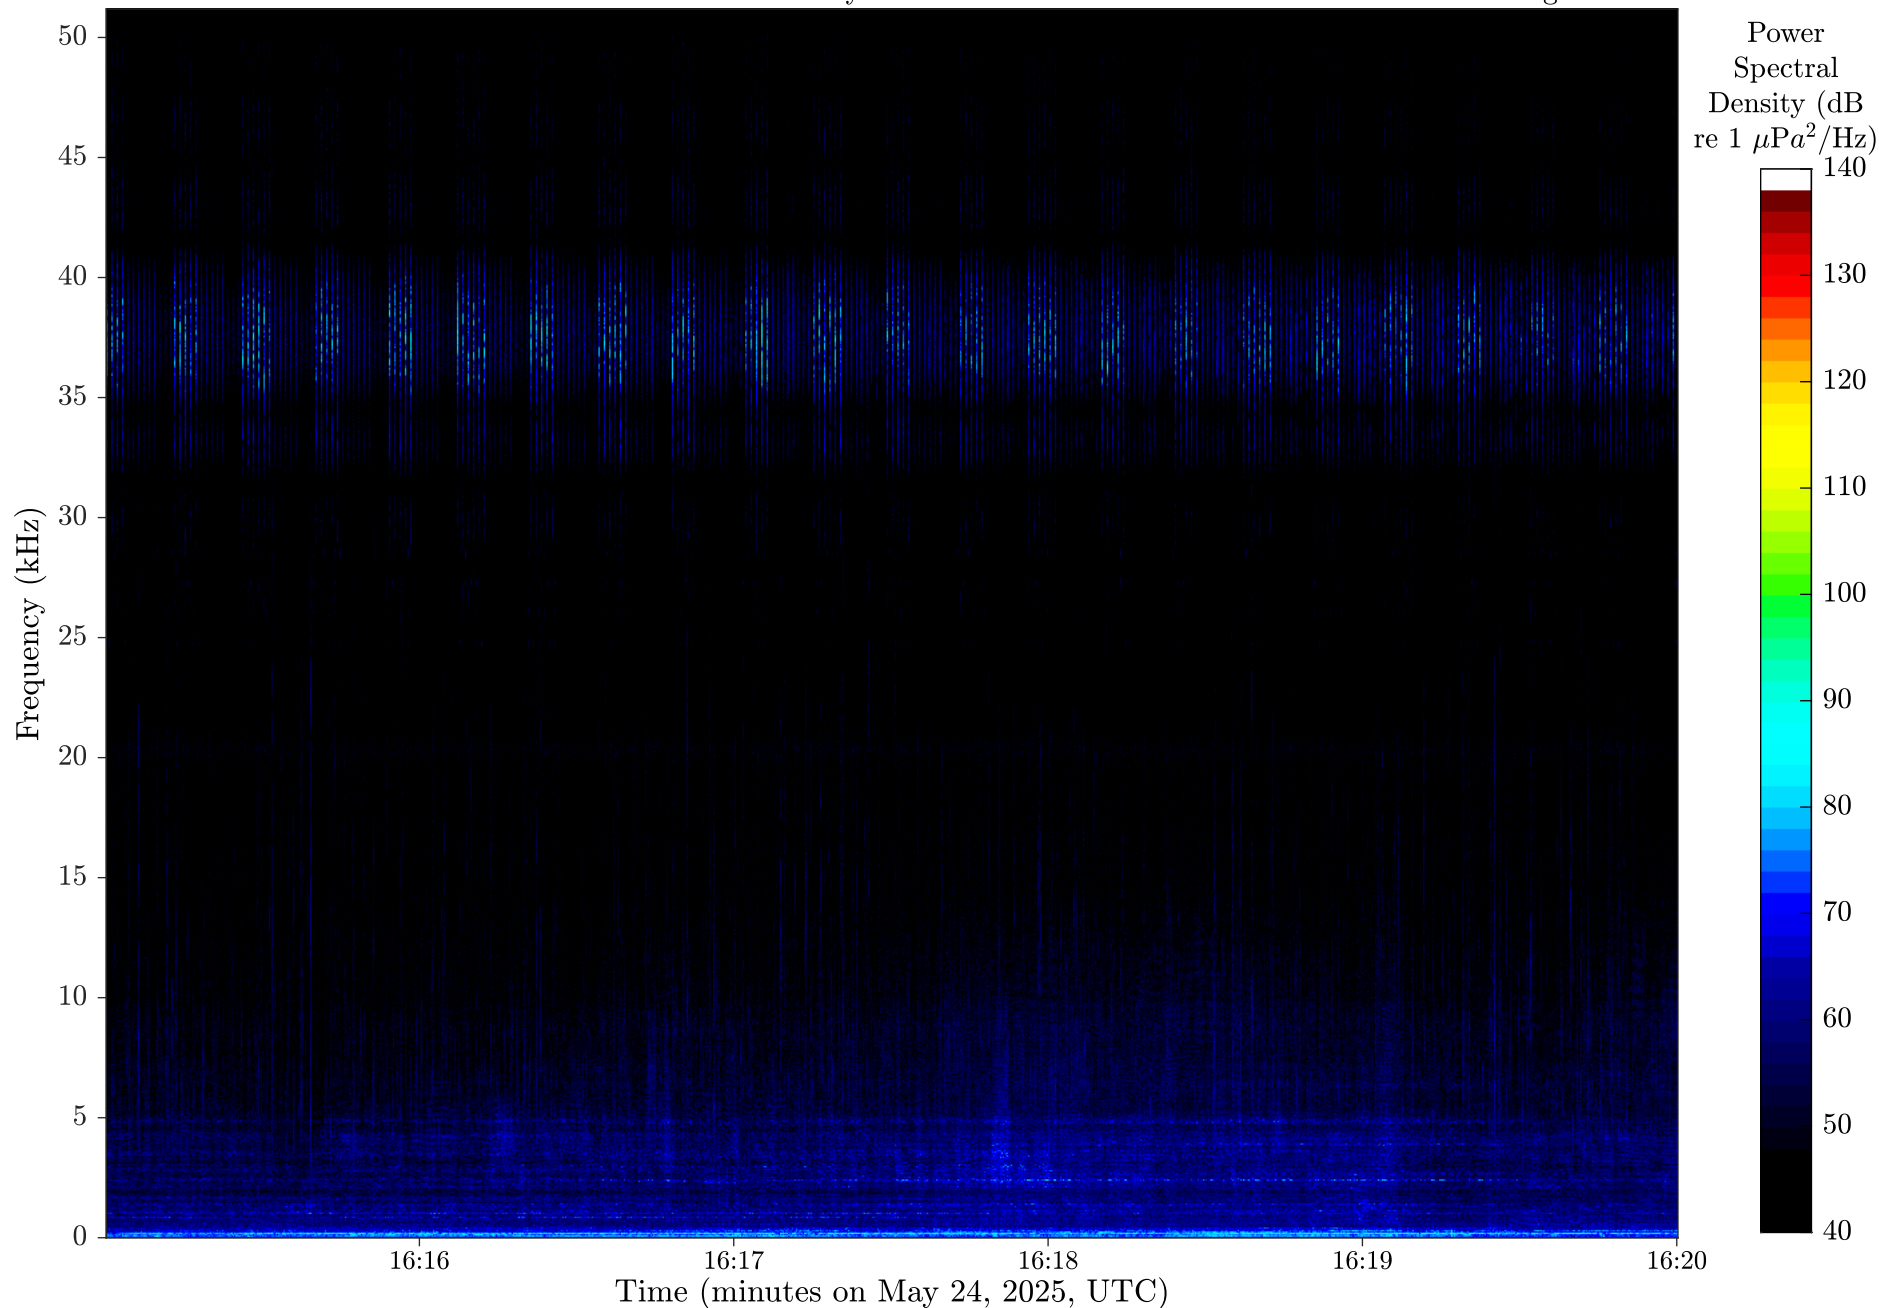


Comments: 29.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:07 UTC

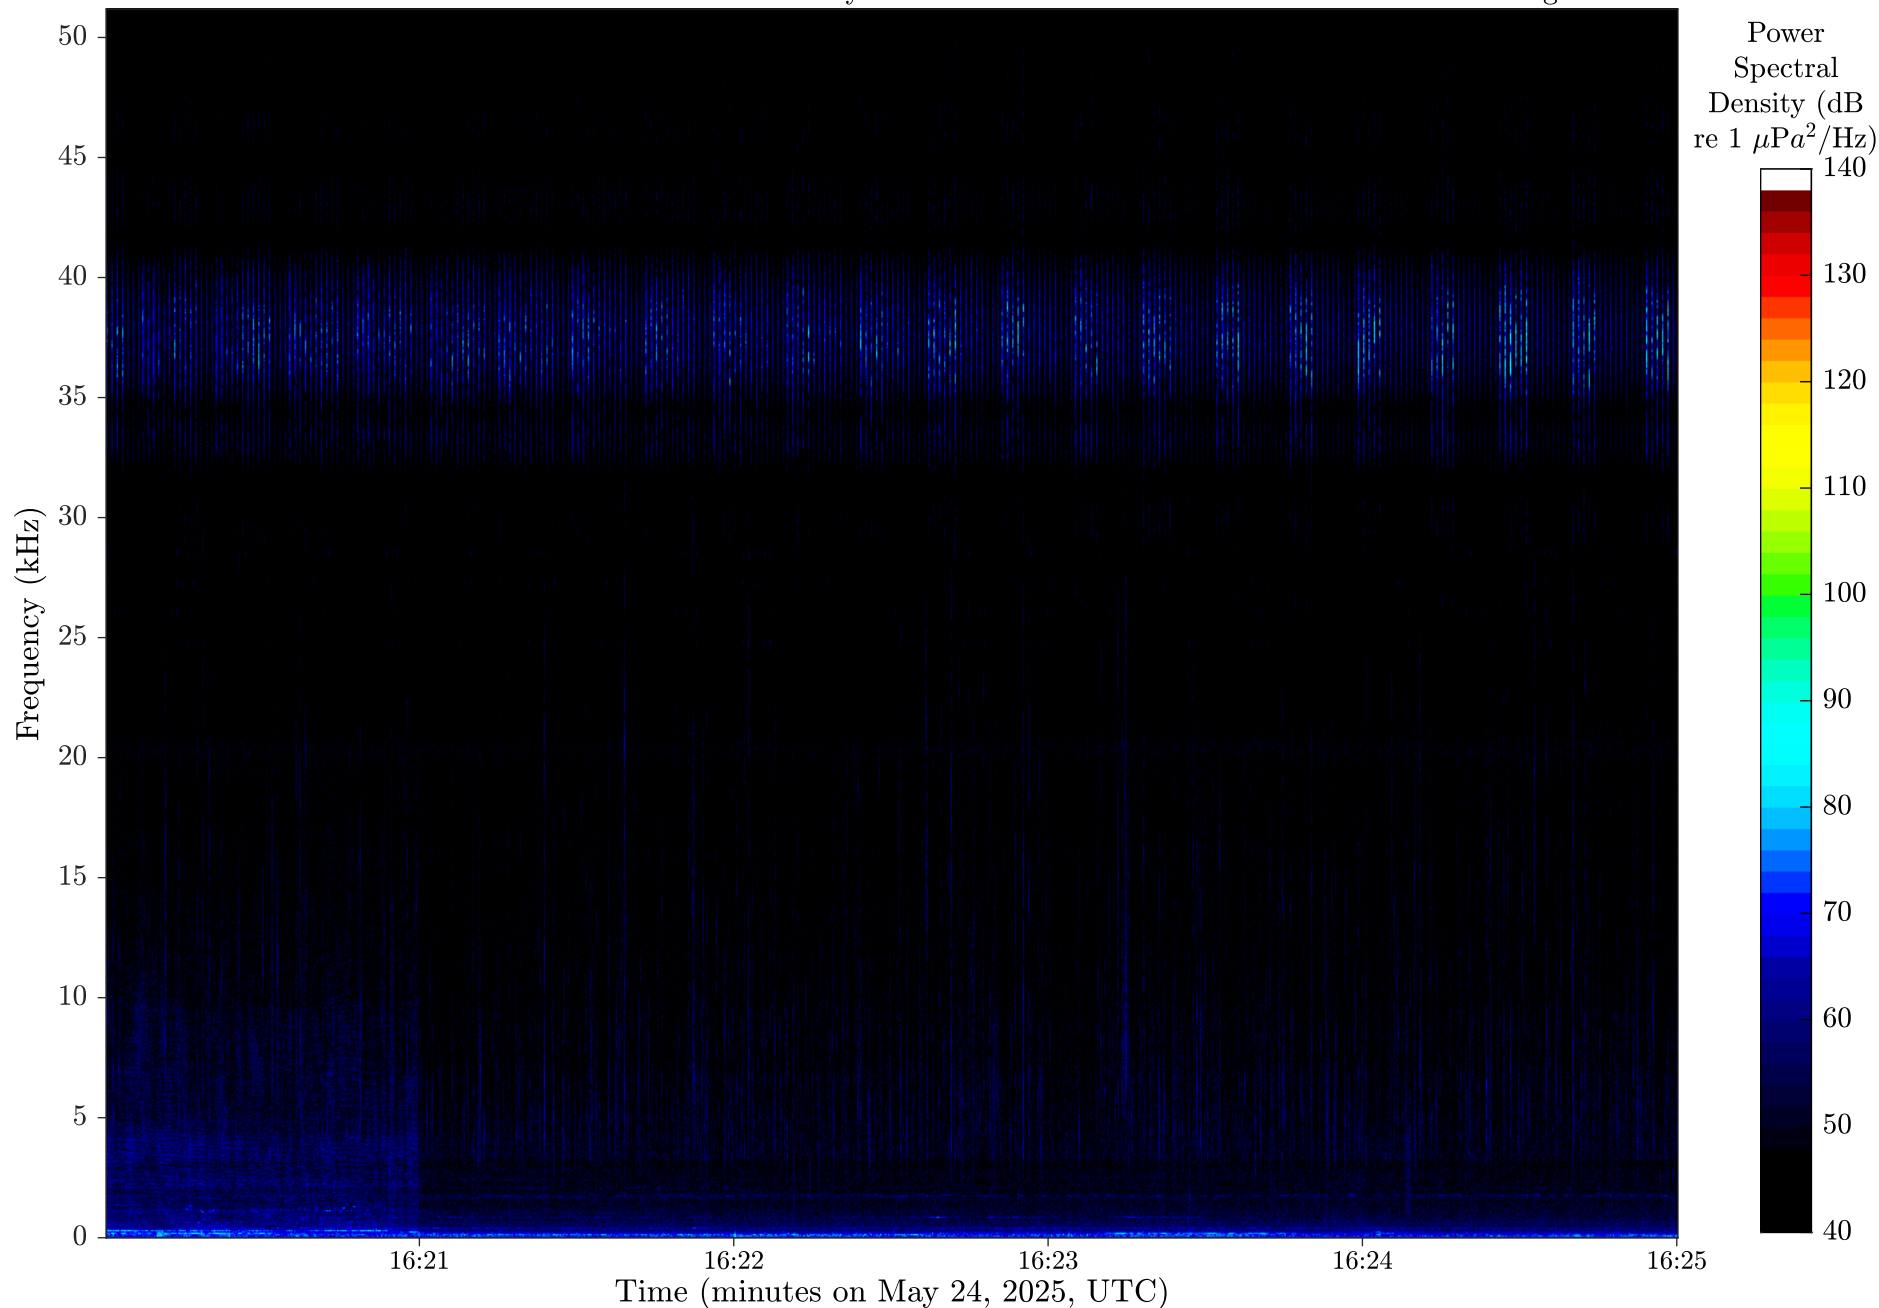


Comments: 29.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:16 UTC

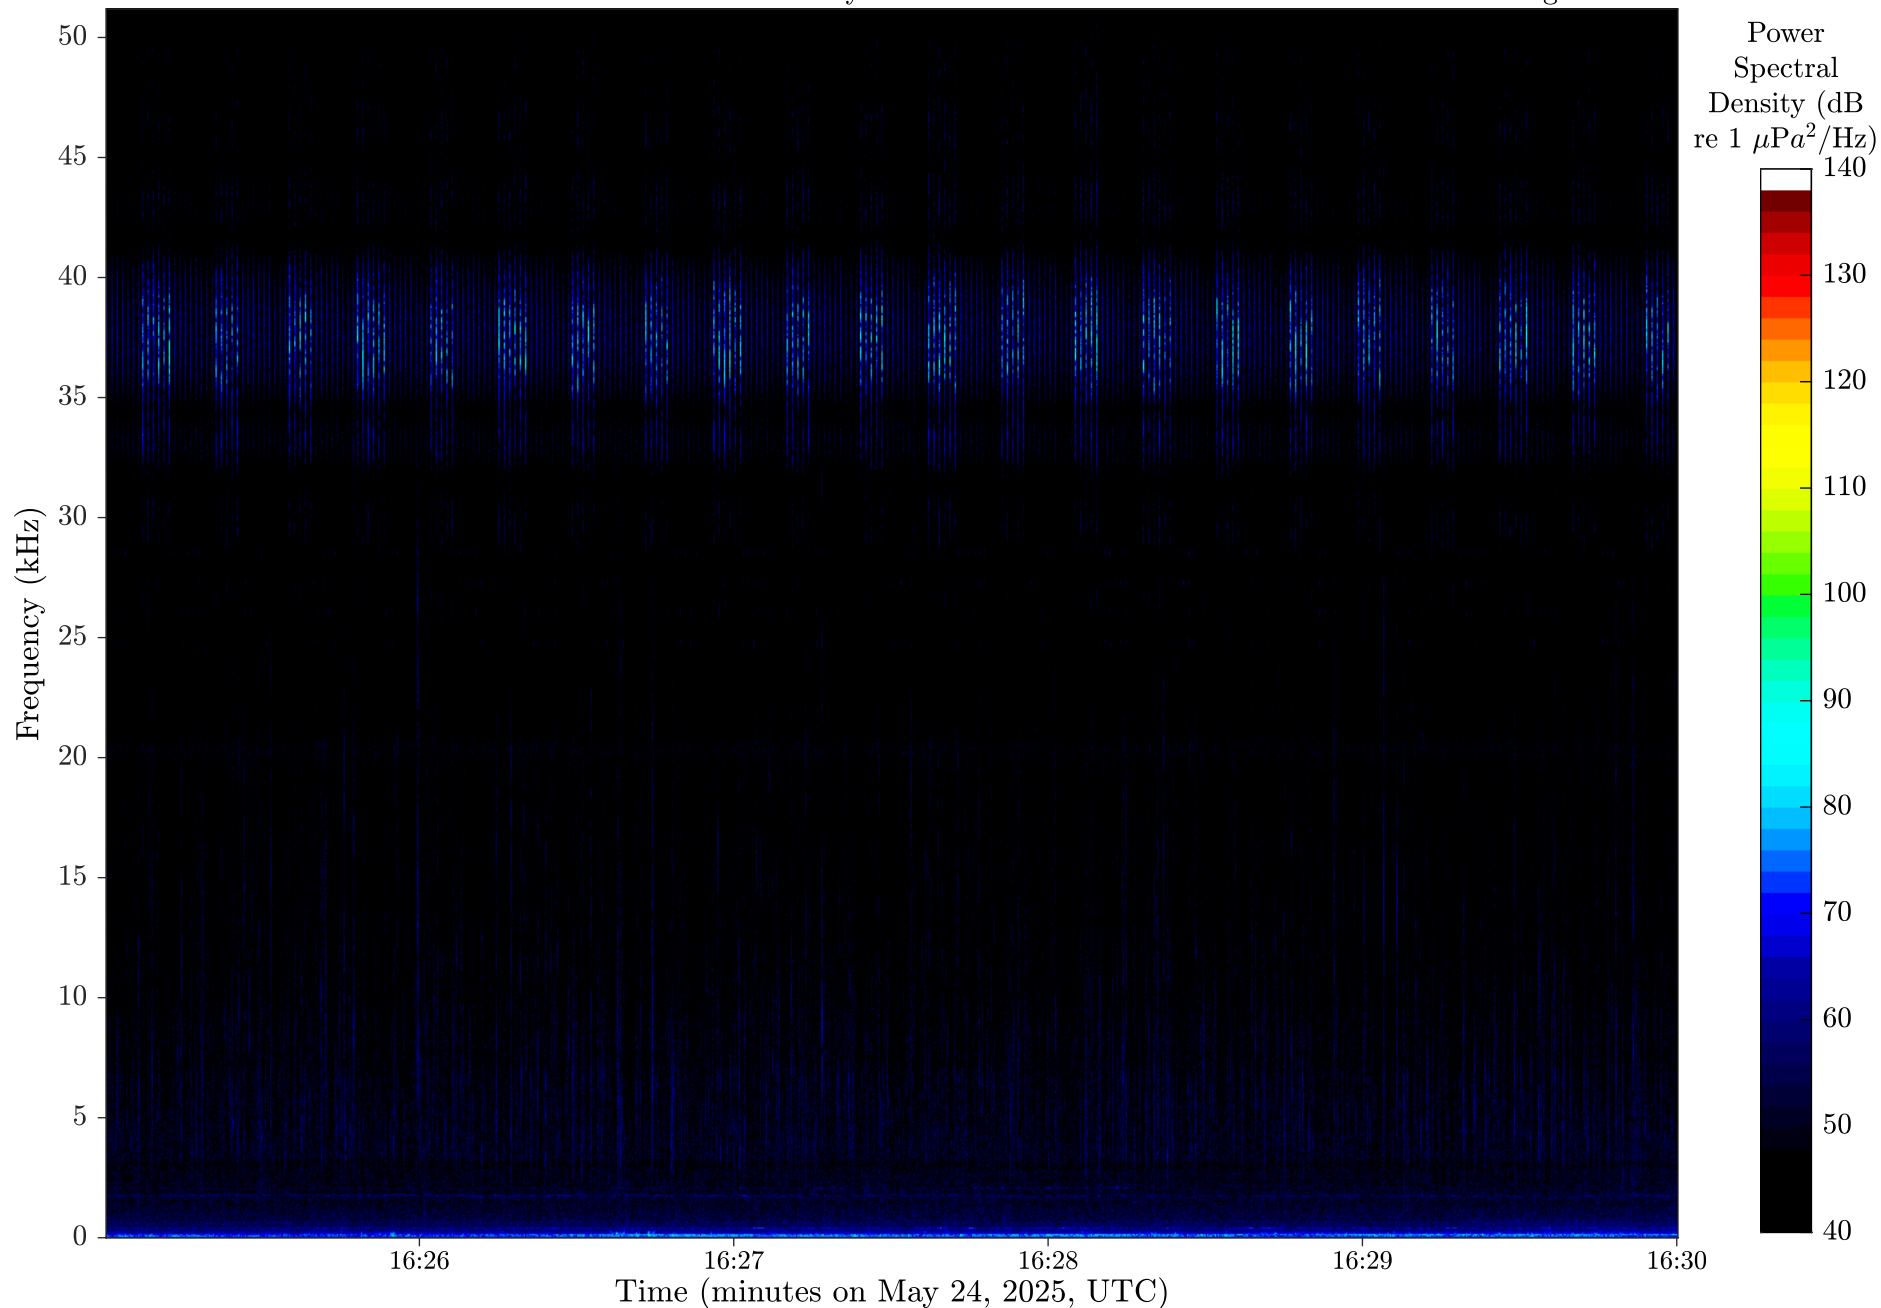


Comments: 29.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:24 UTC

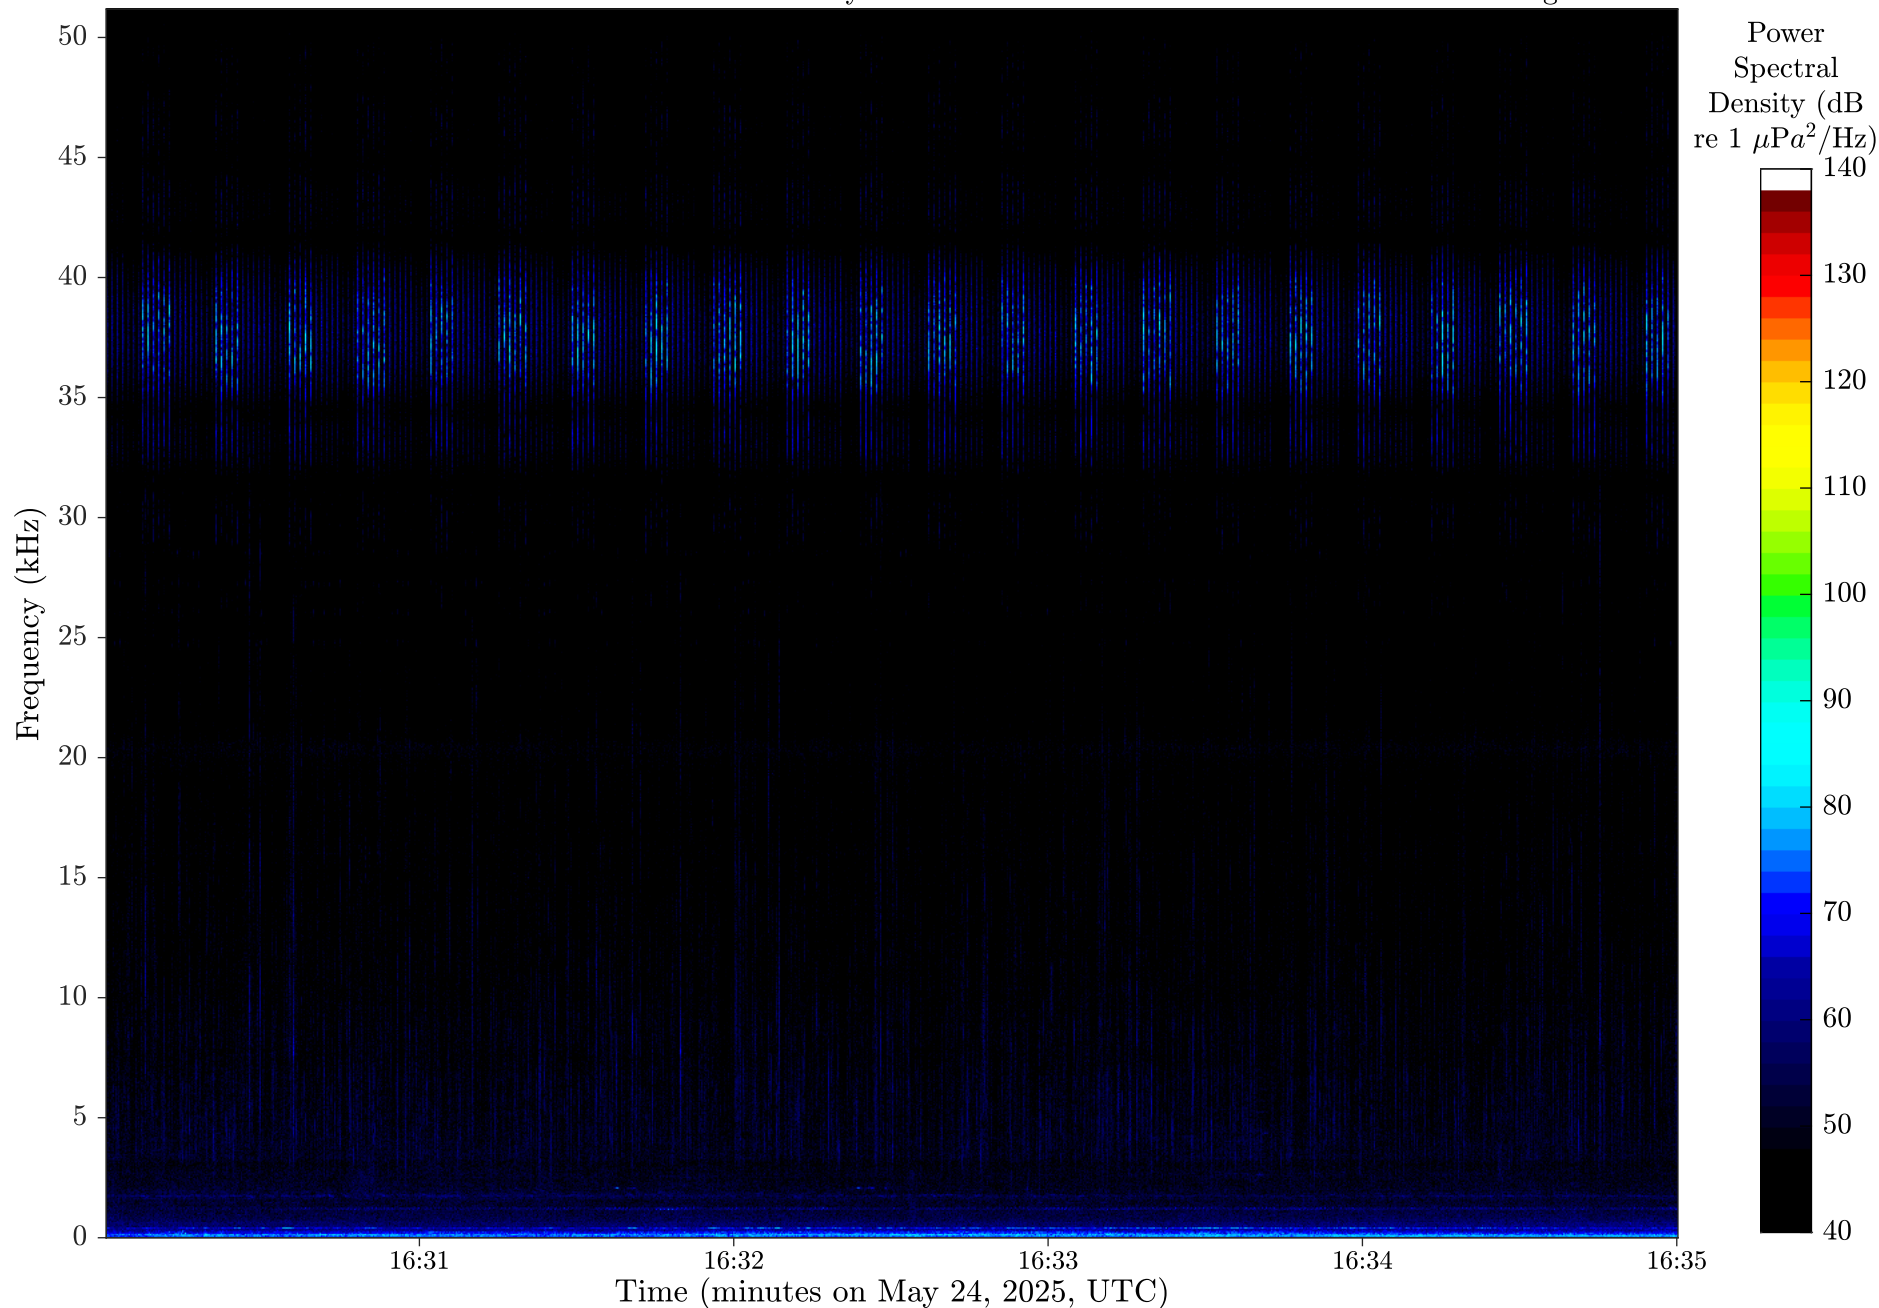


Comments: 31.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:33 UTC

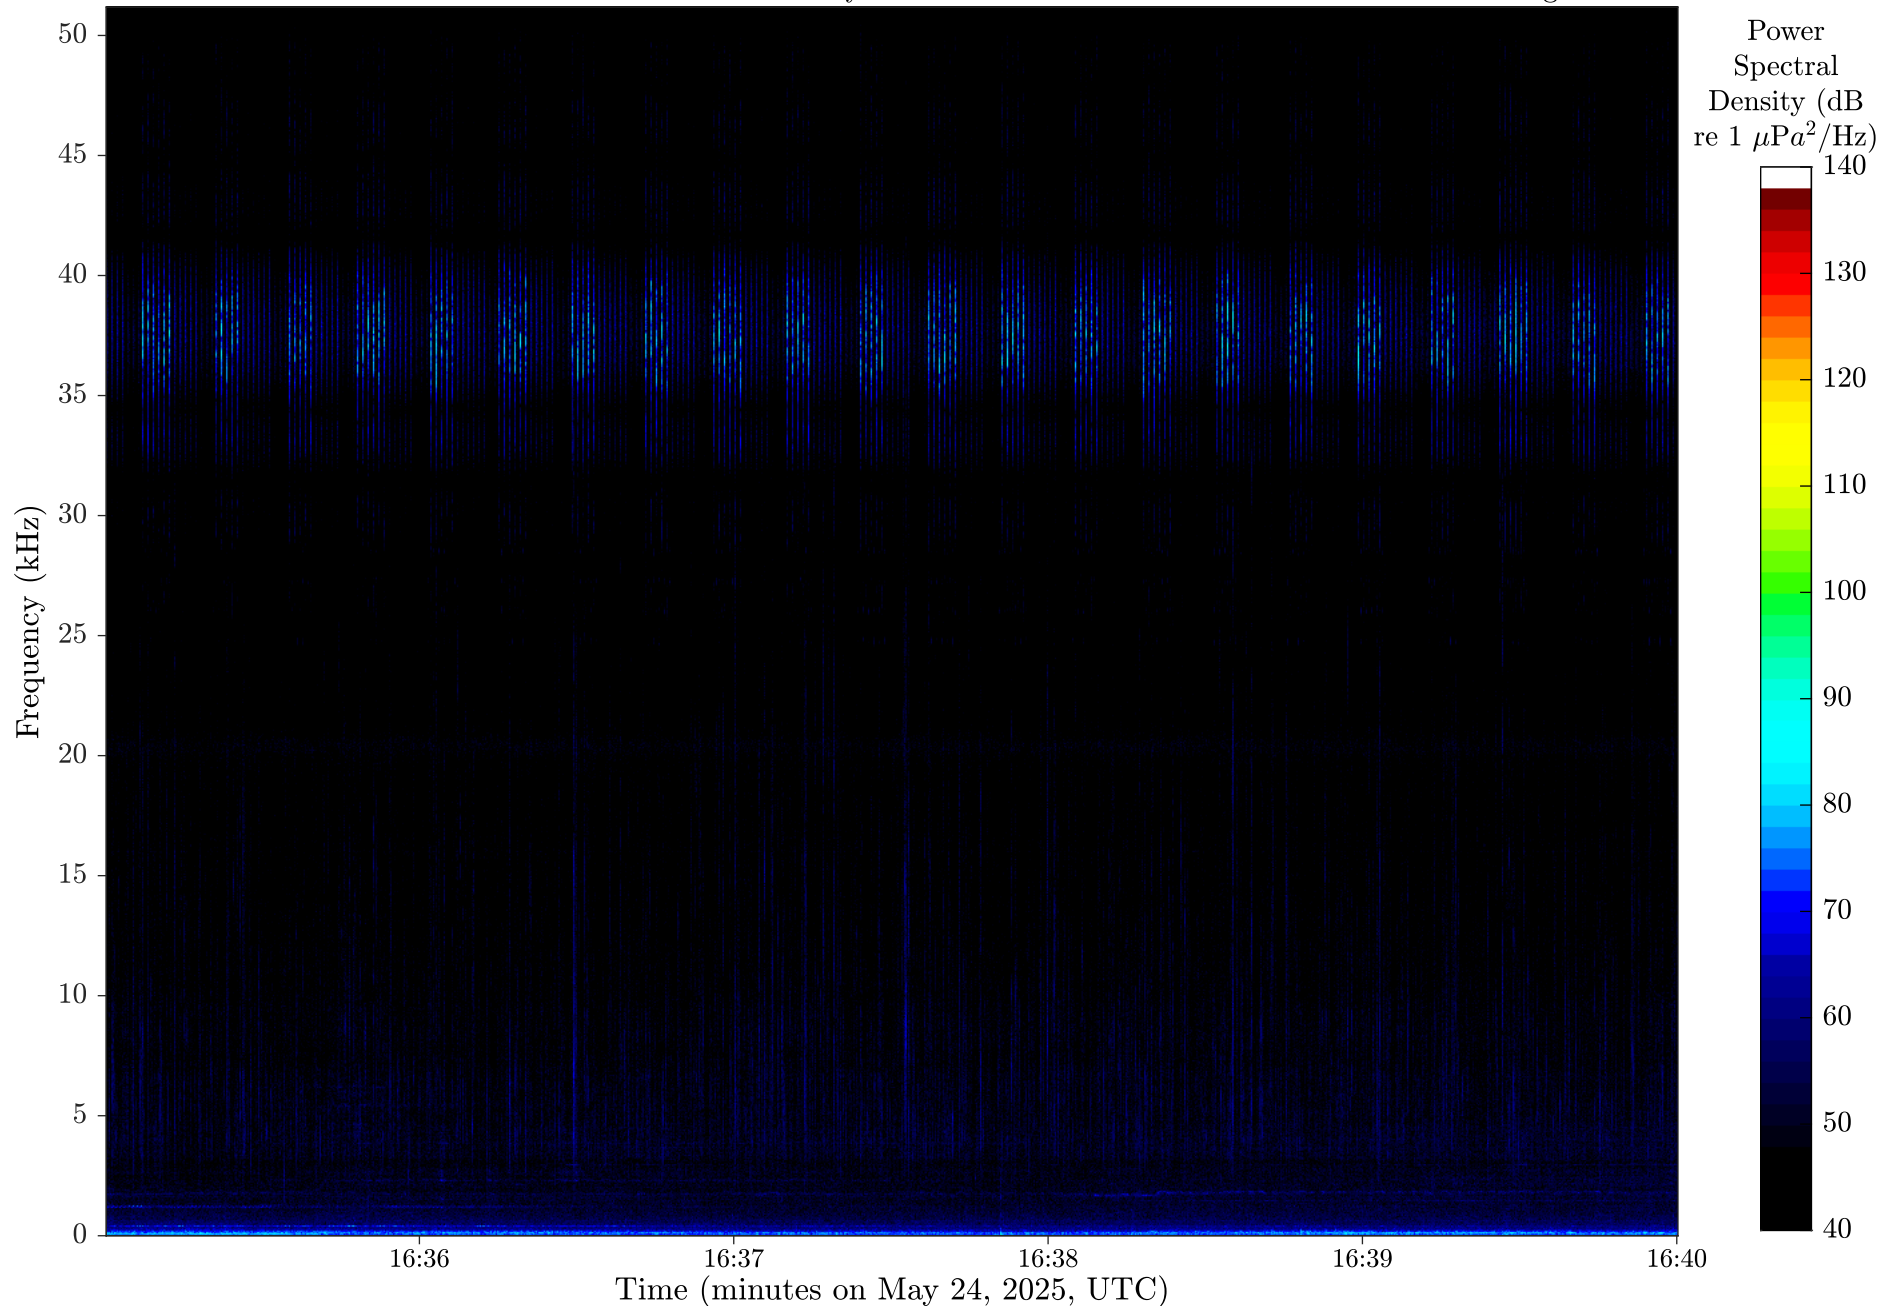


Comments: 30.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:41 UTC

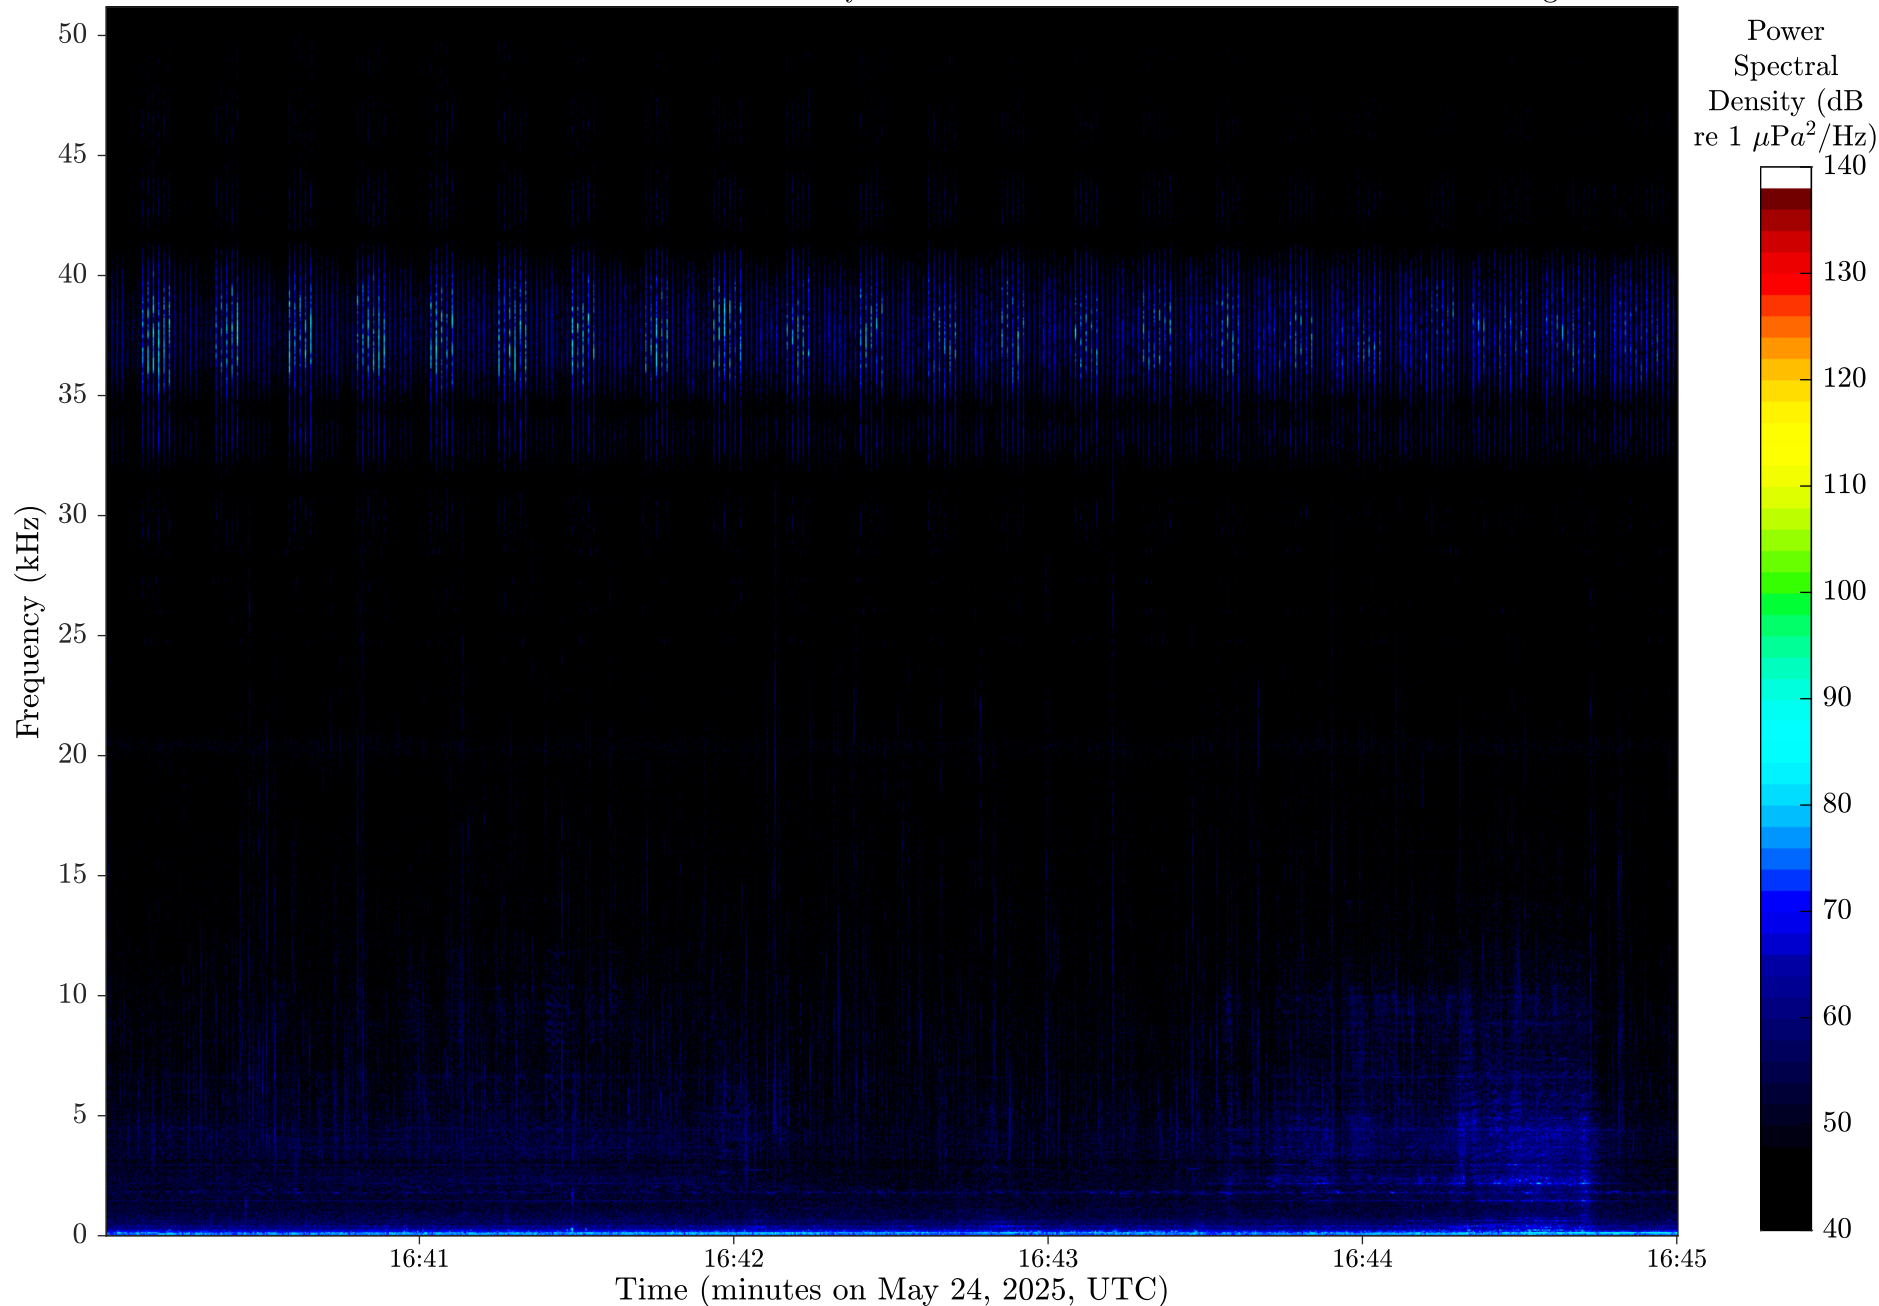


Comments: 29.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:42:49 UTC

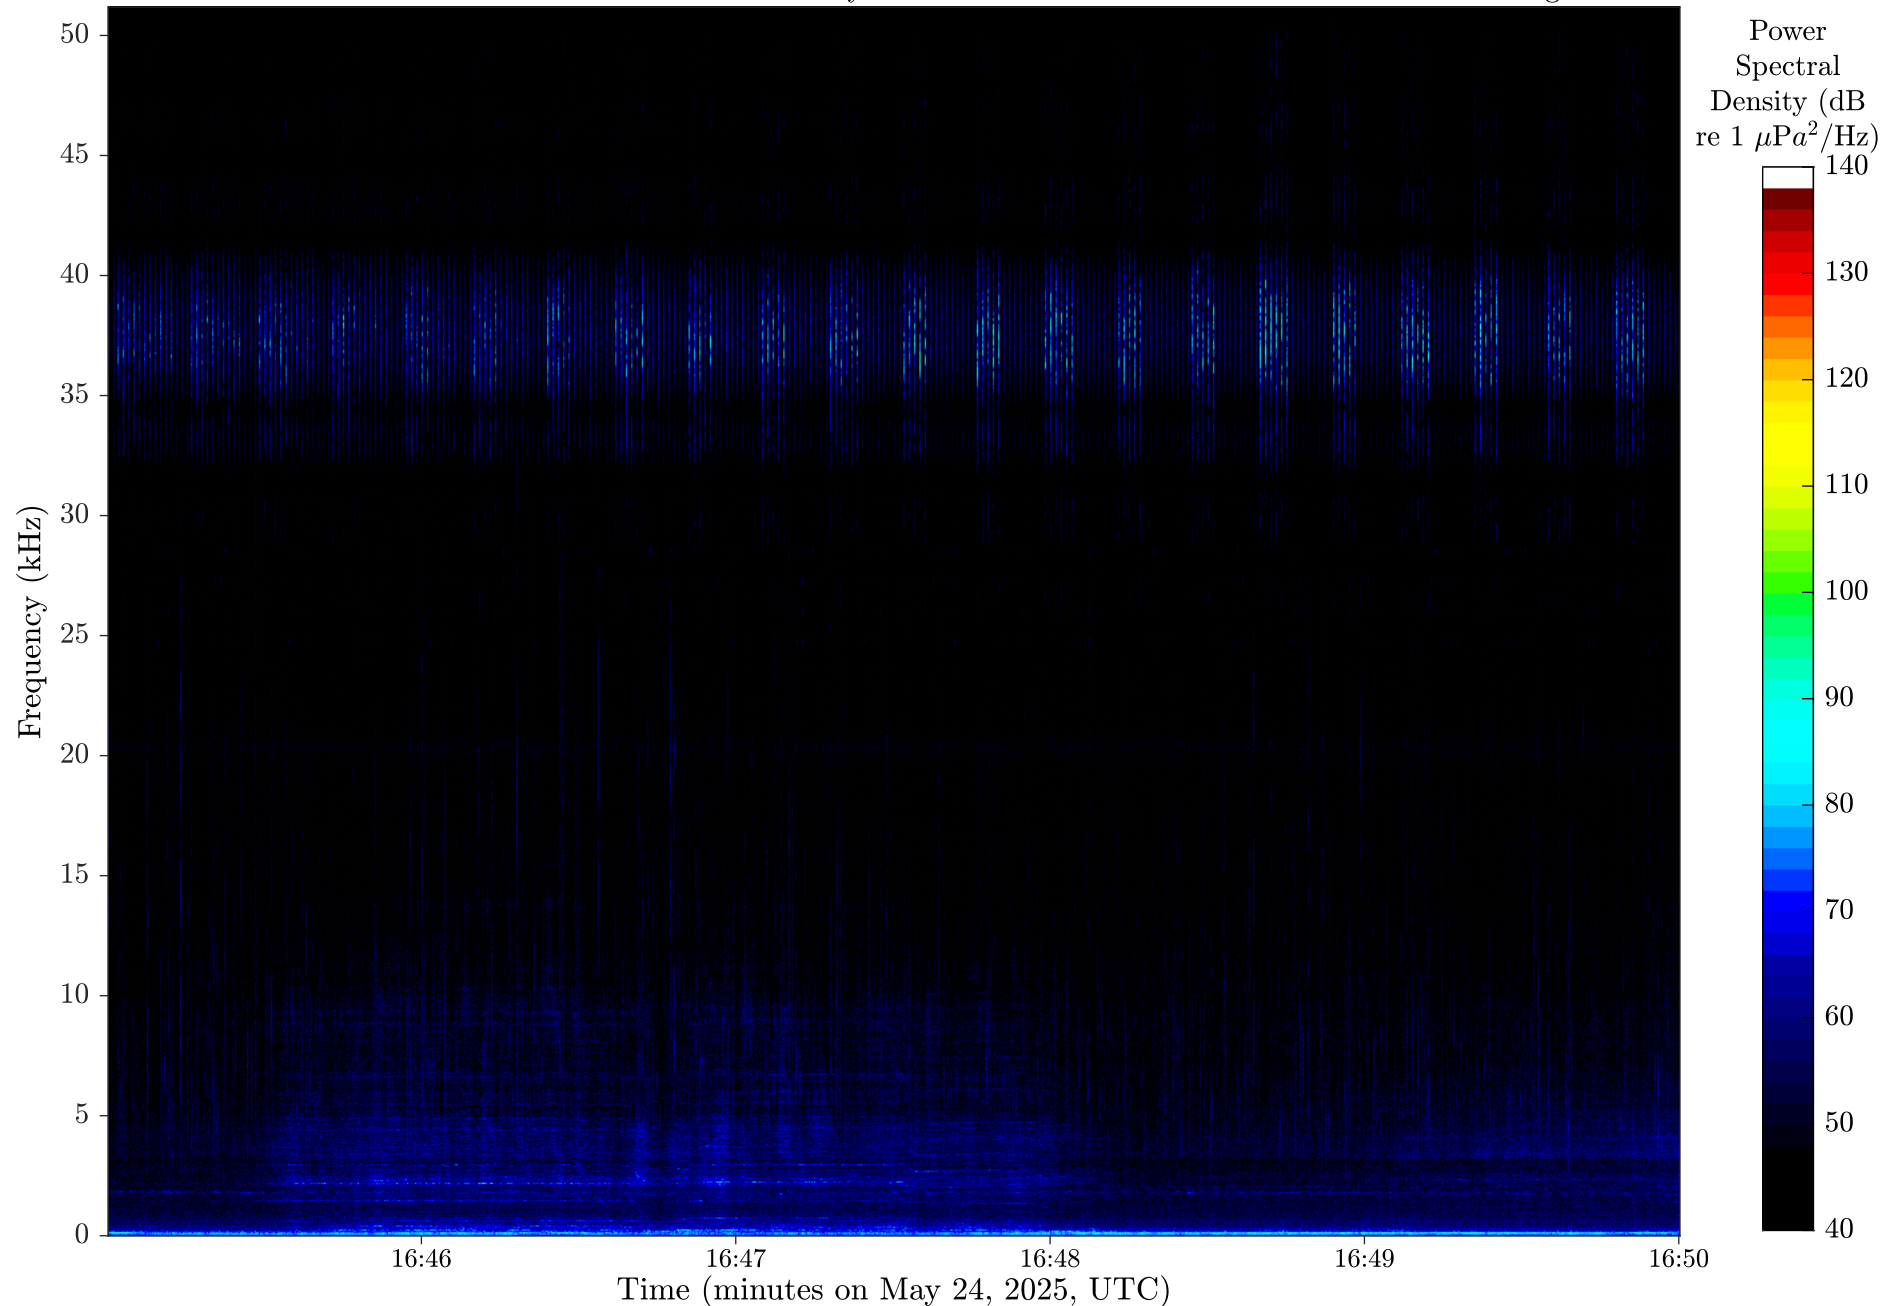

Comments: 29.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:42:58 UTC

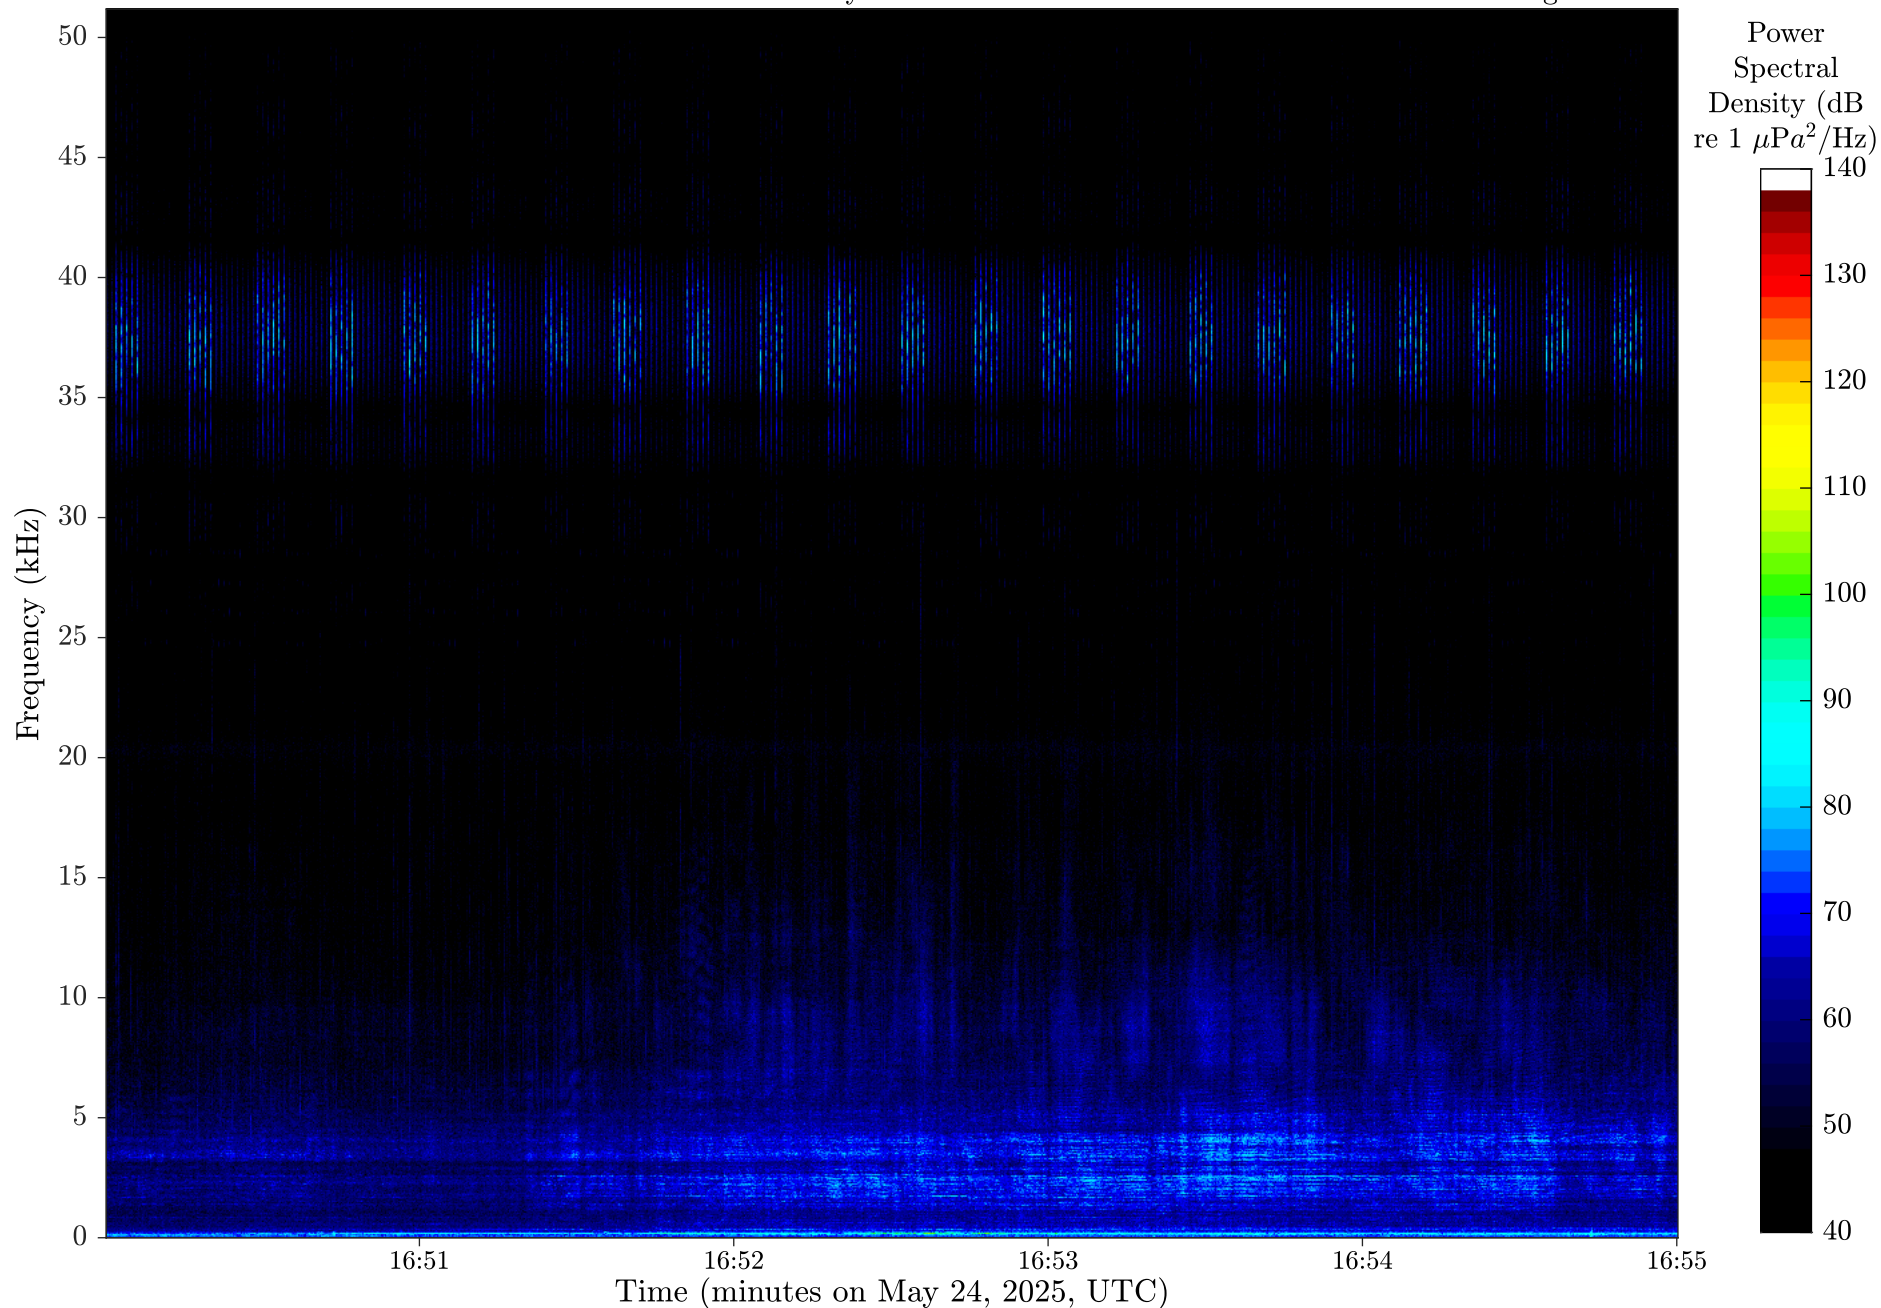

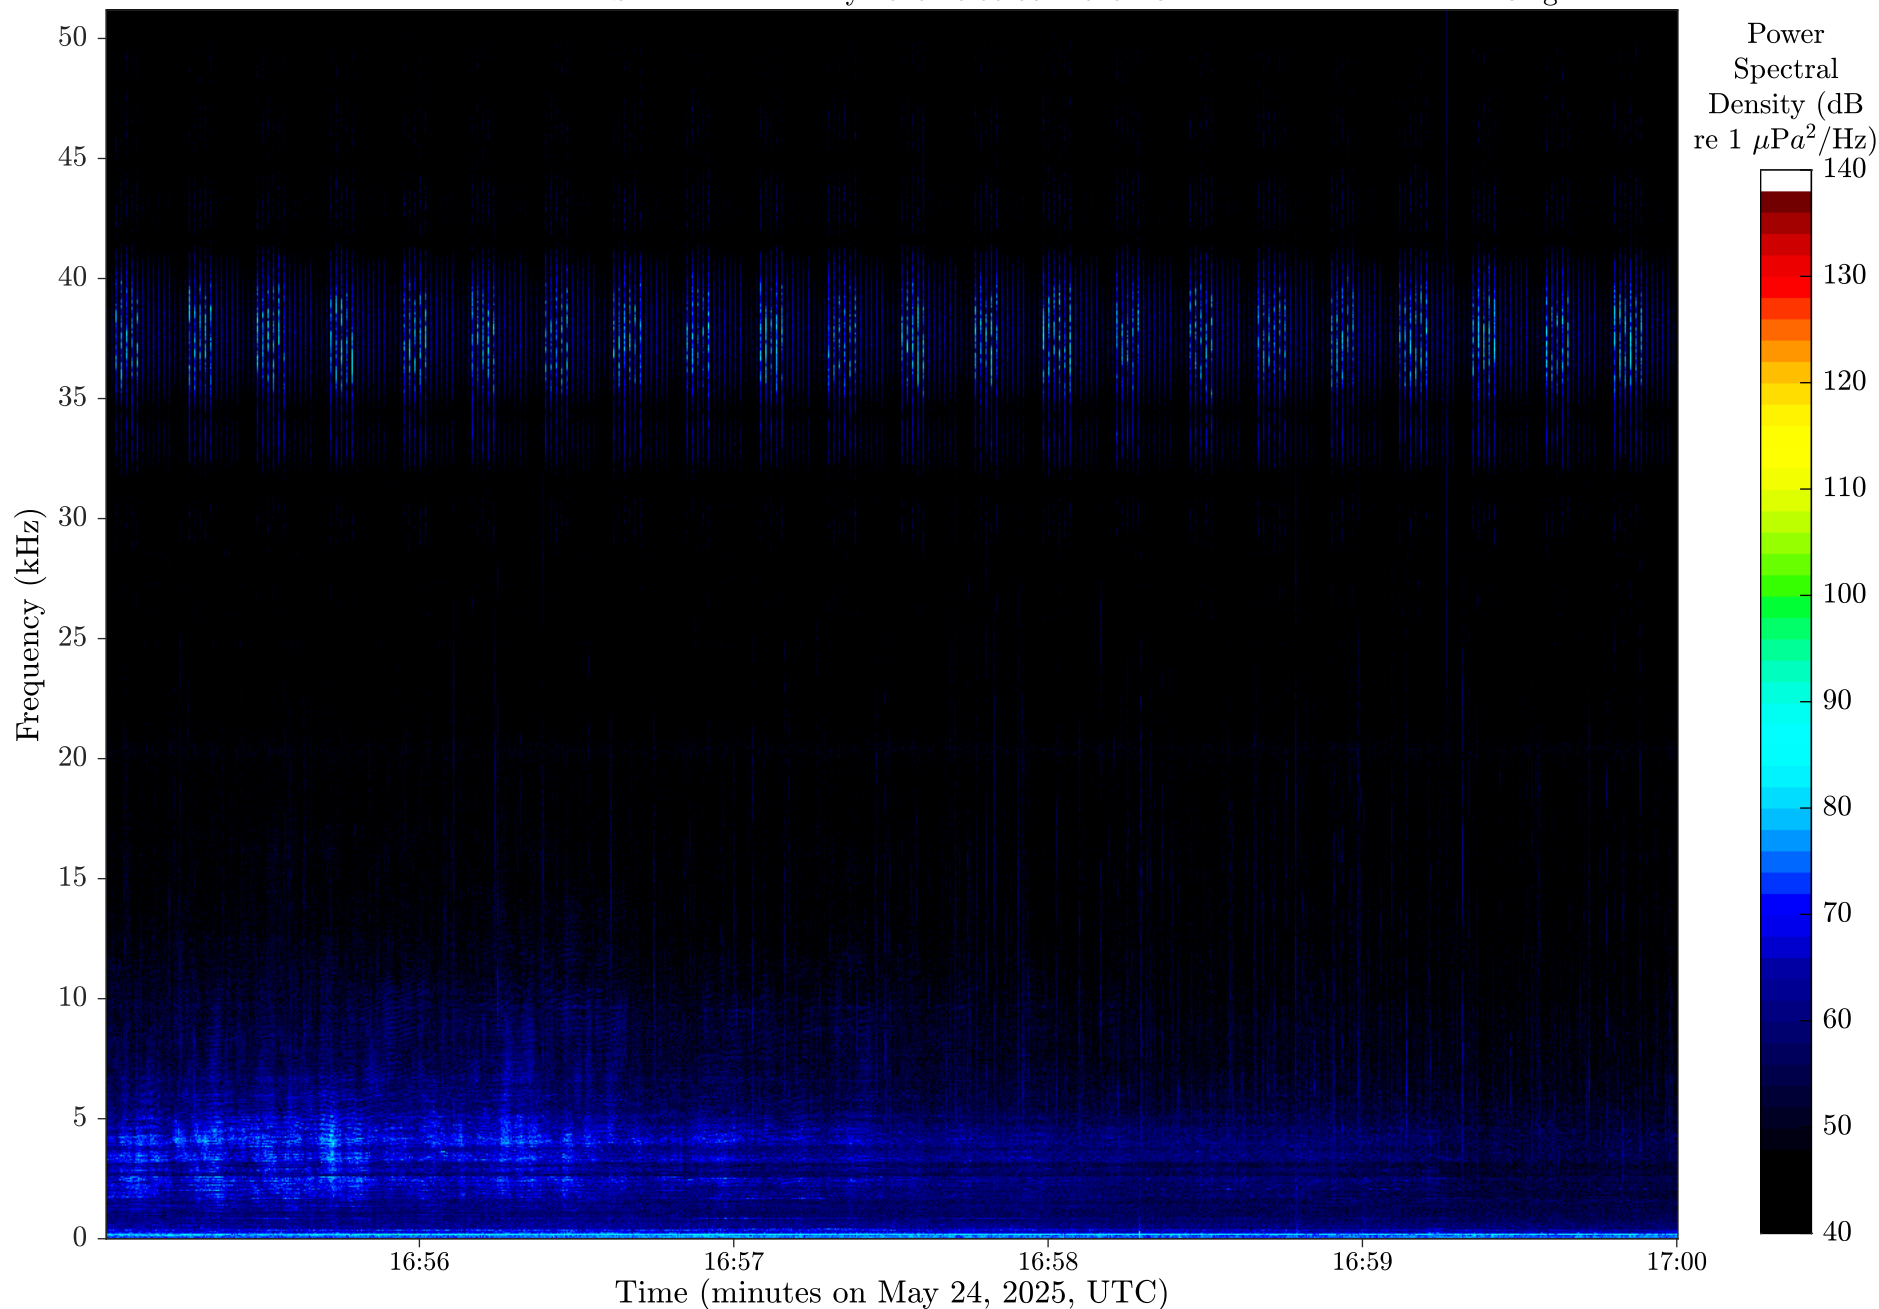


Comments: 28.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:43:15 UTC

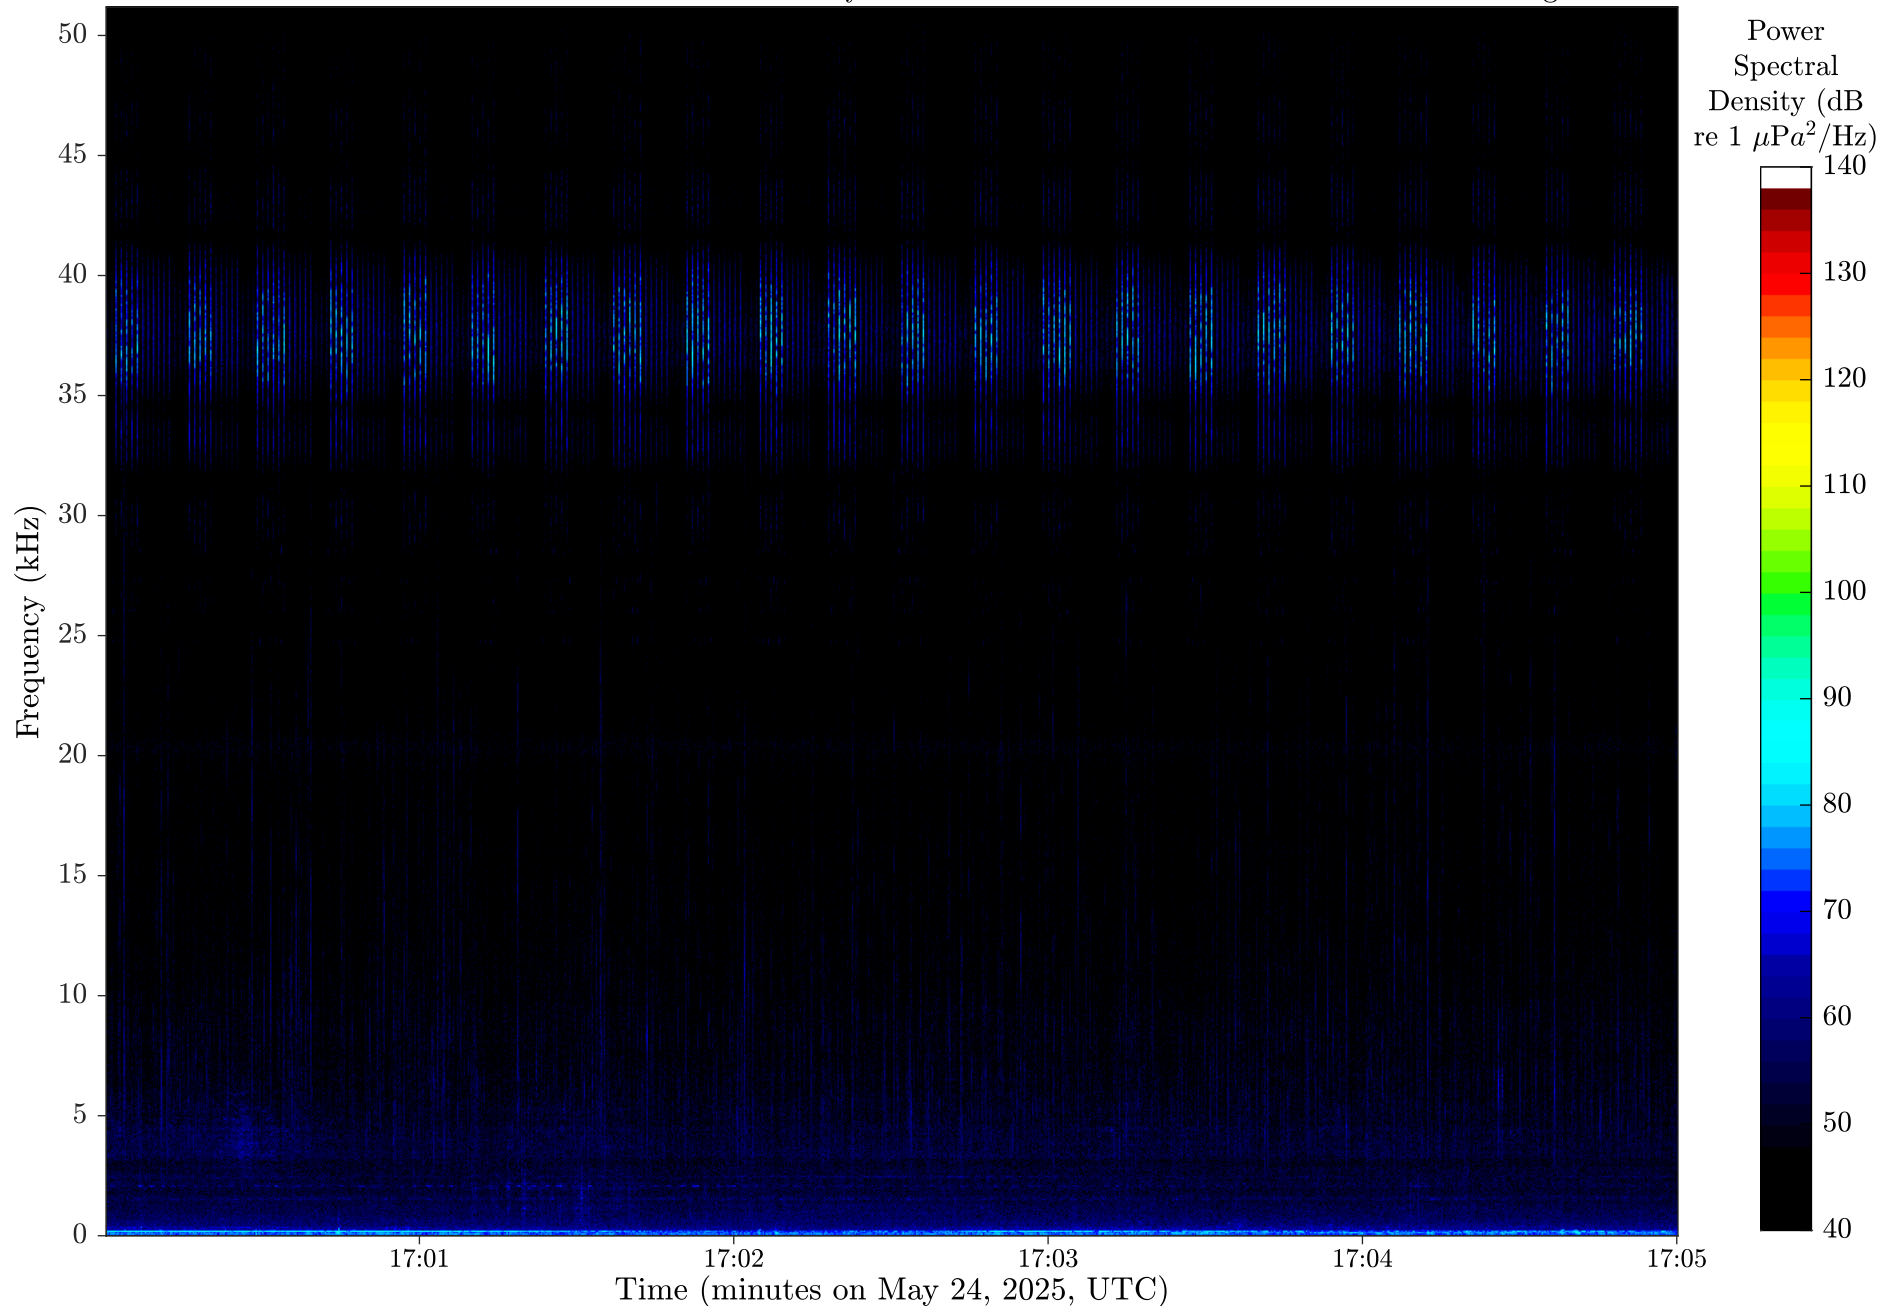


Comments: 28.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:43:23 UTC

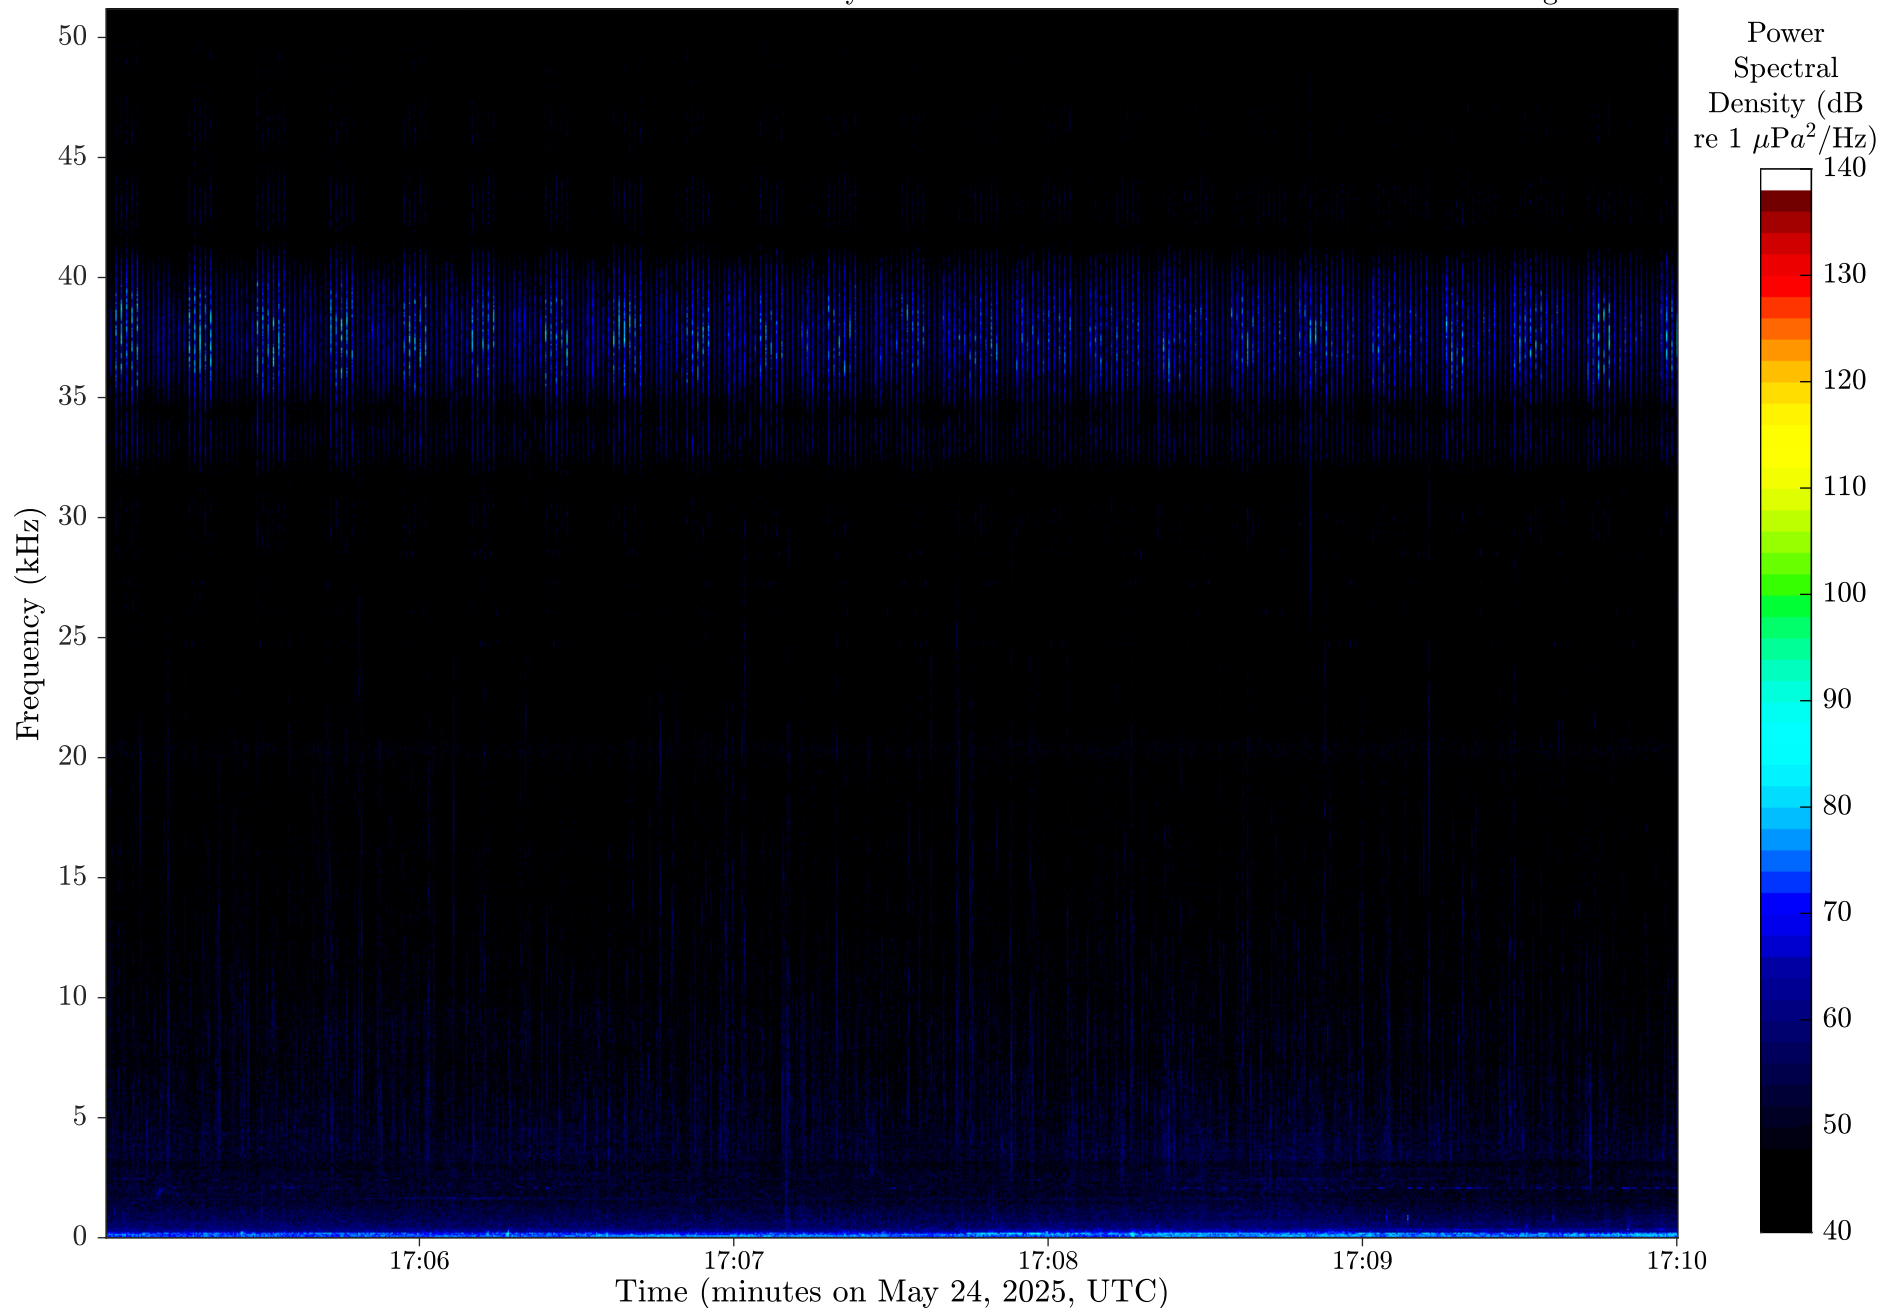


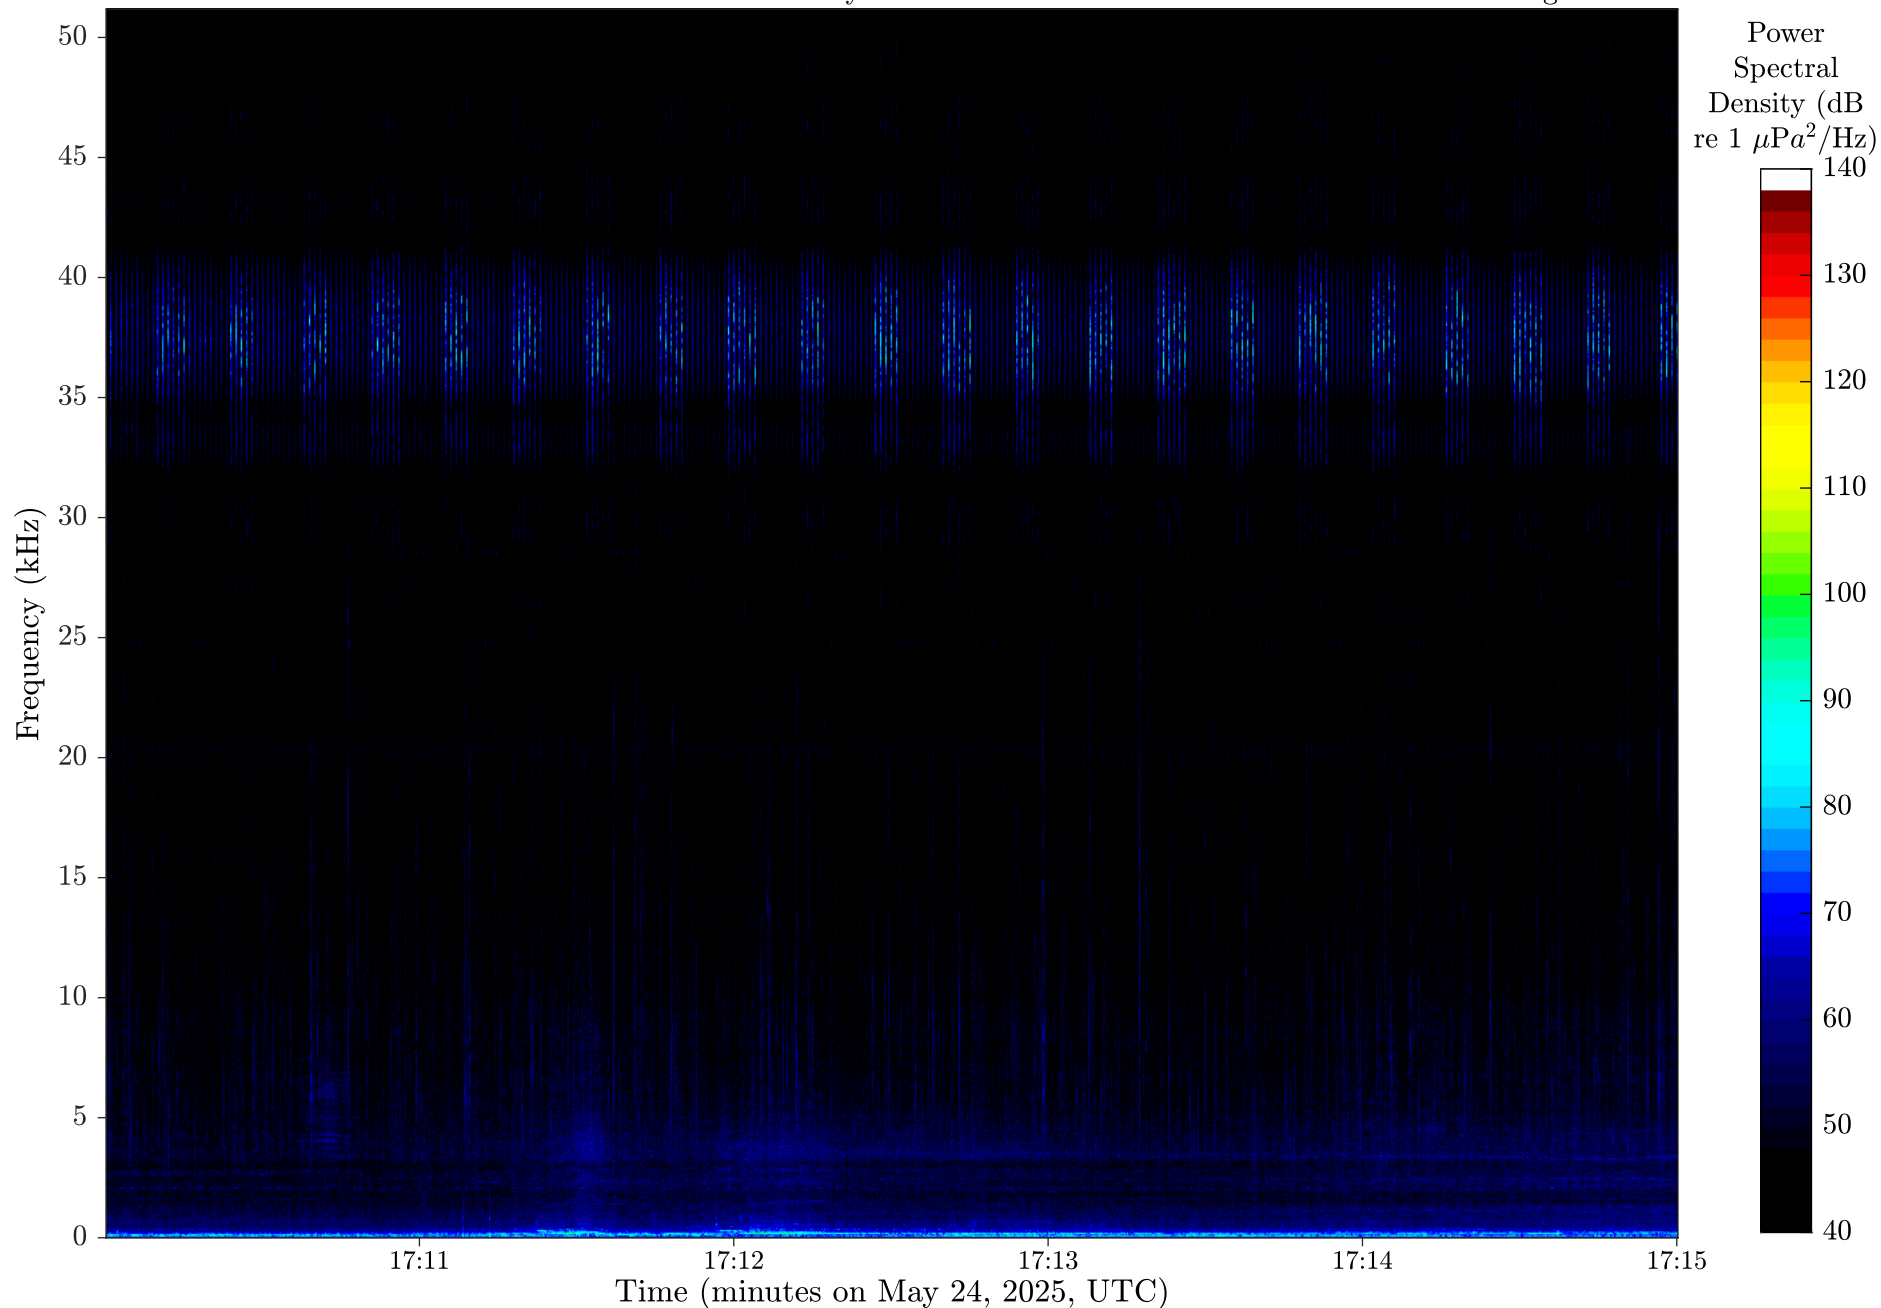

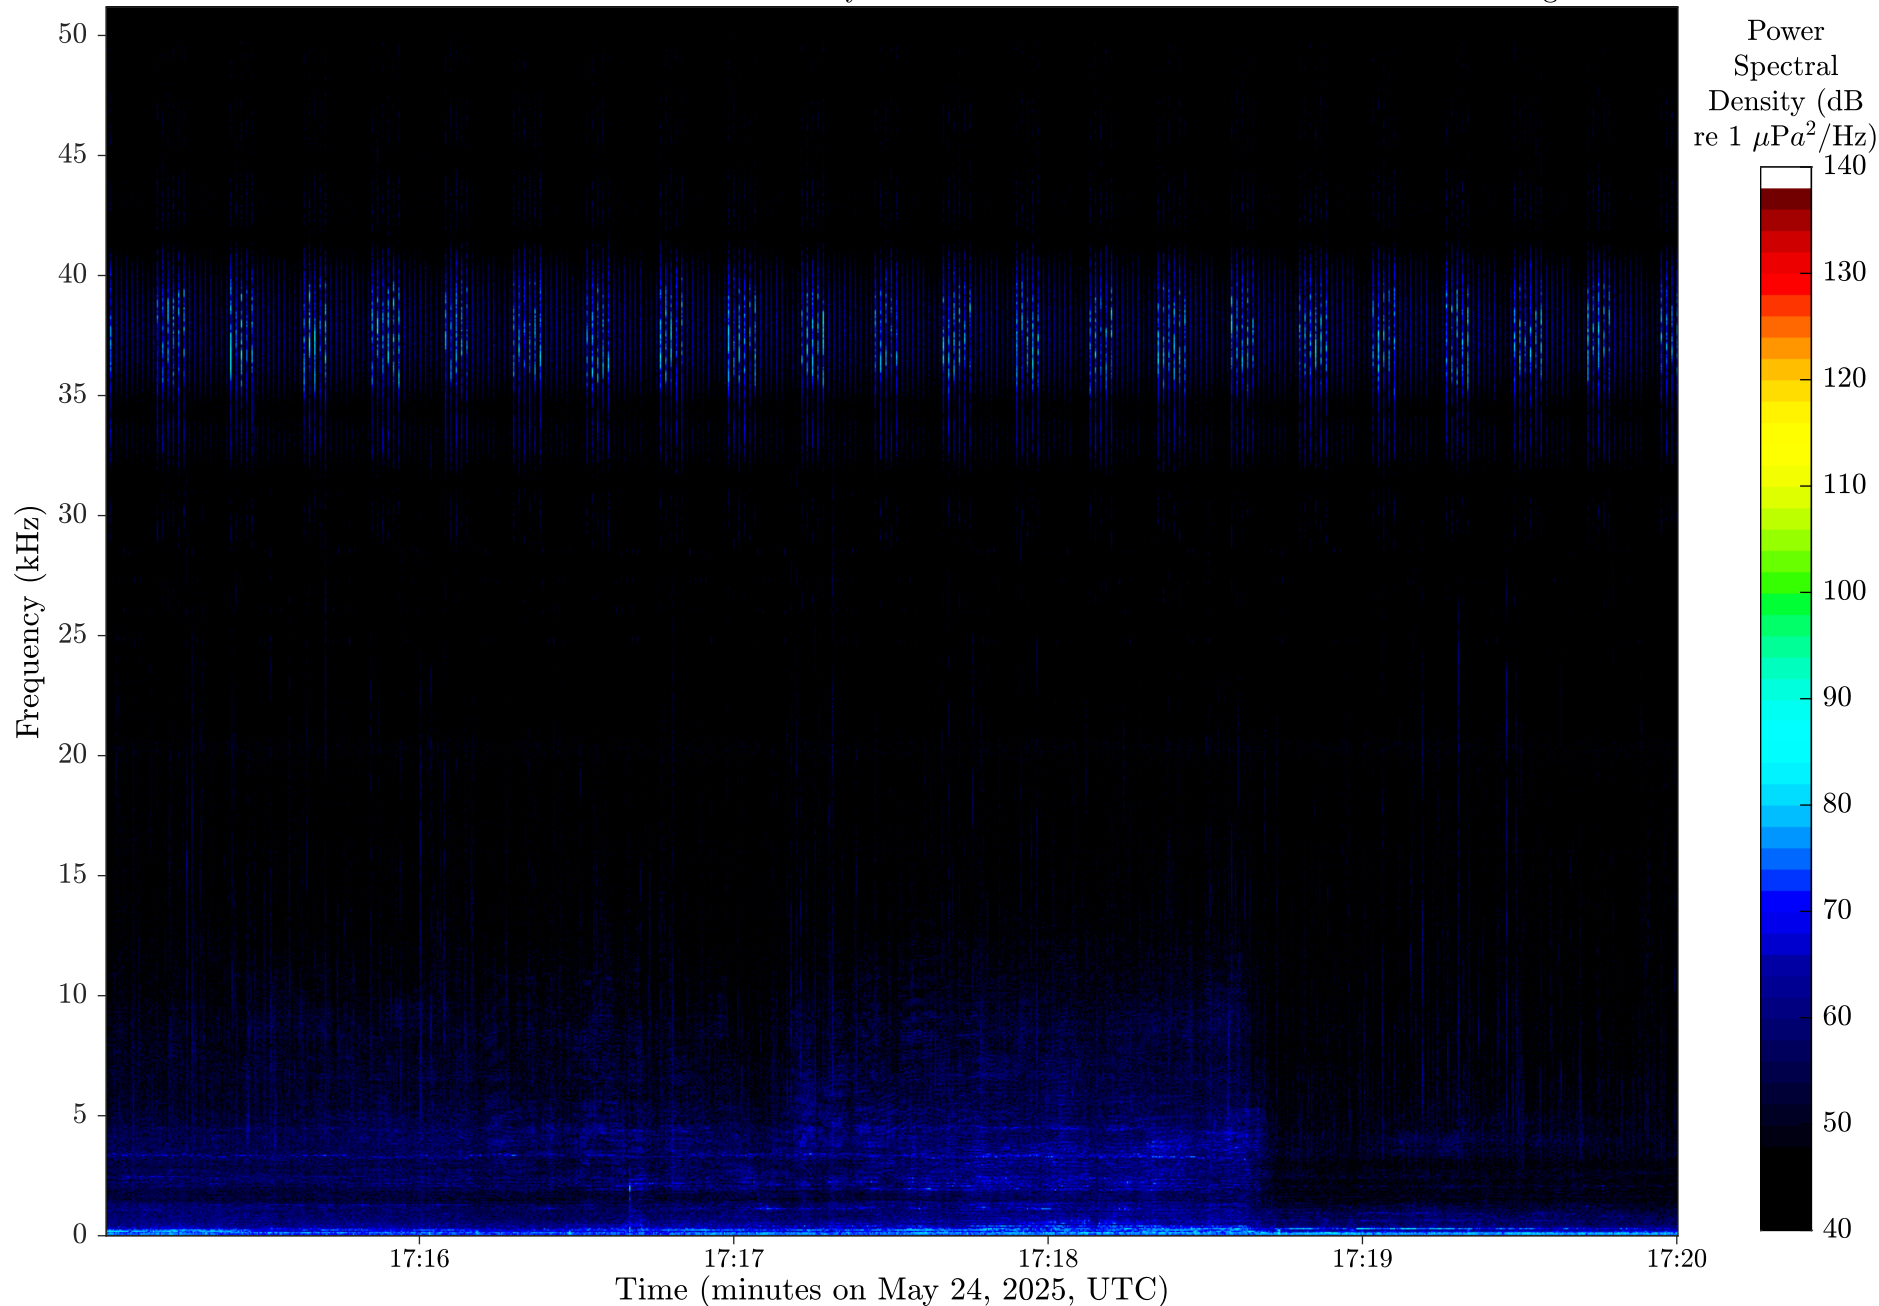


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:43:48 UTC

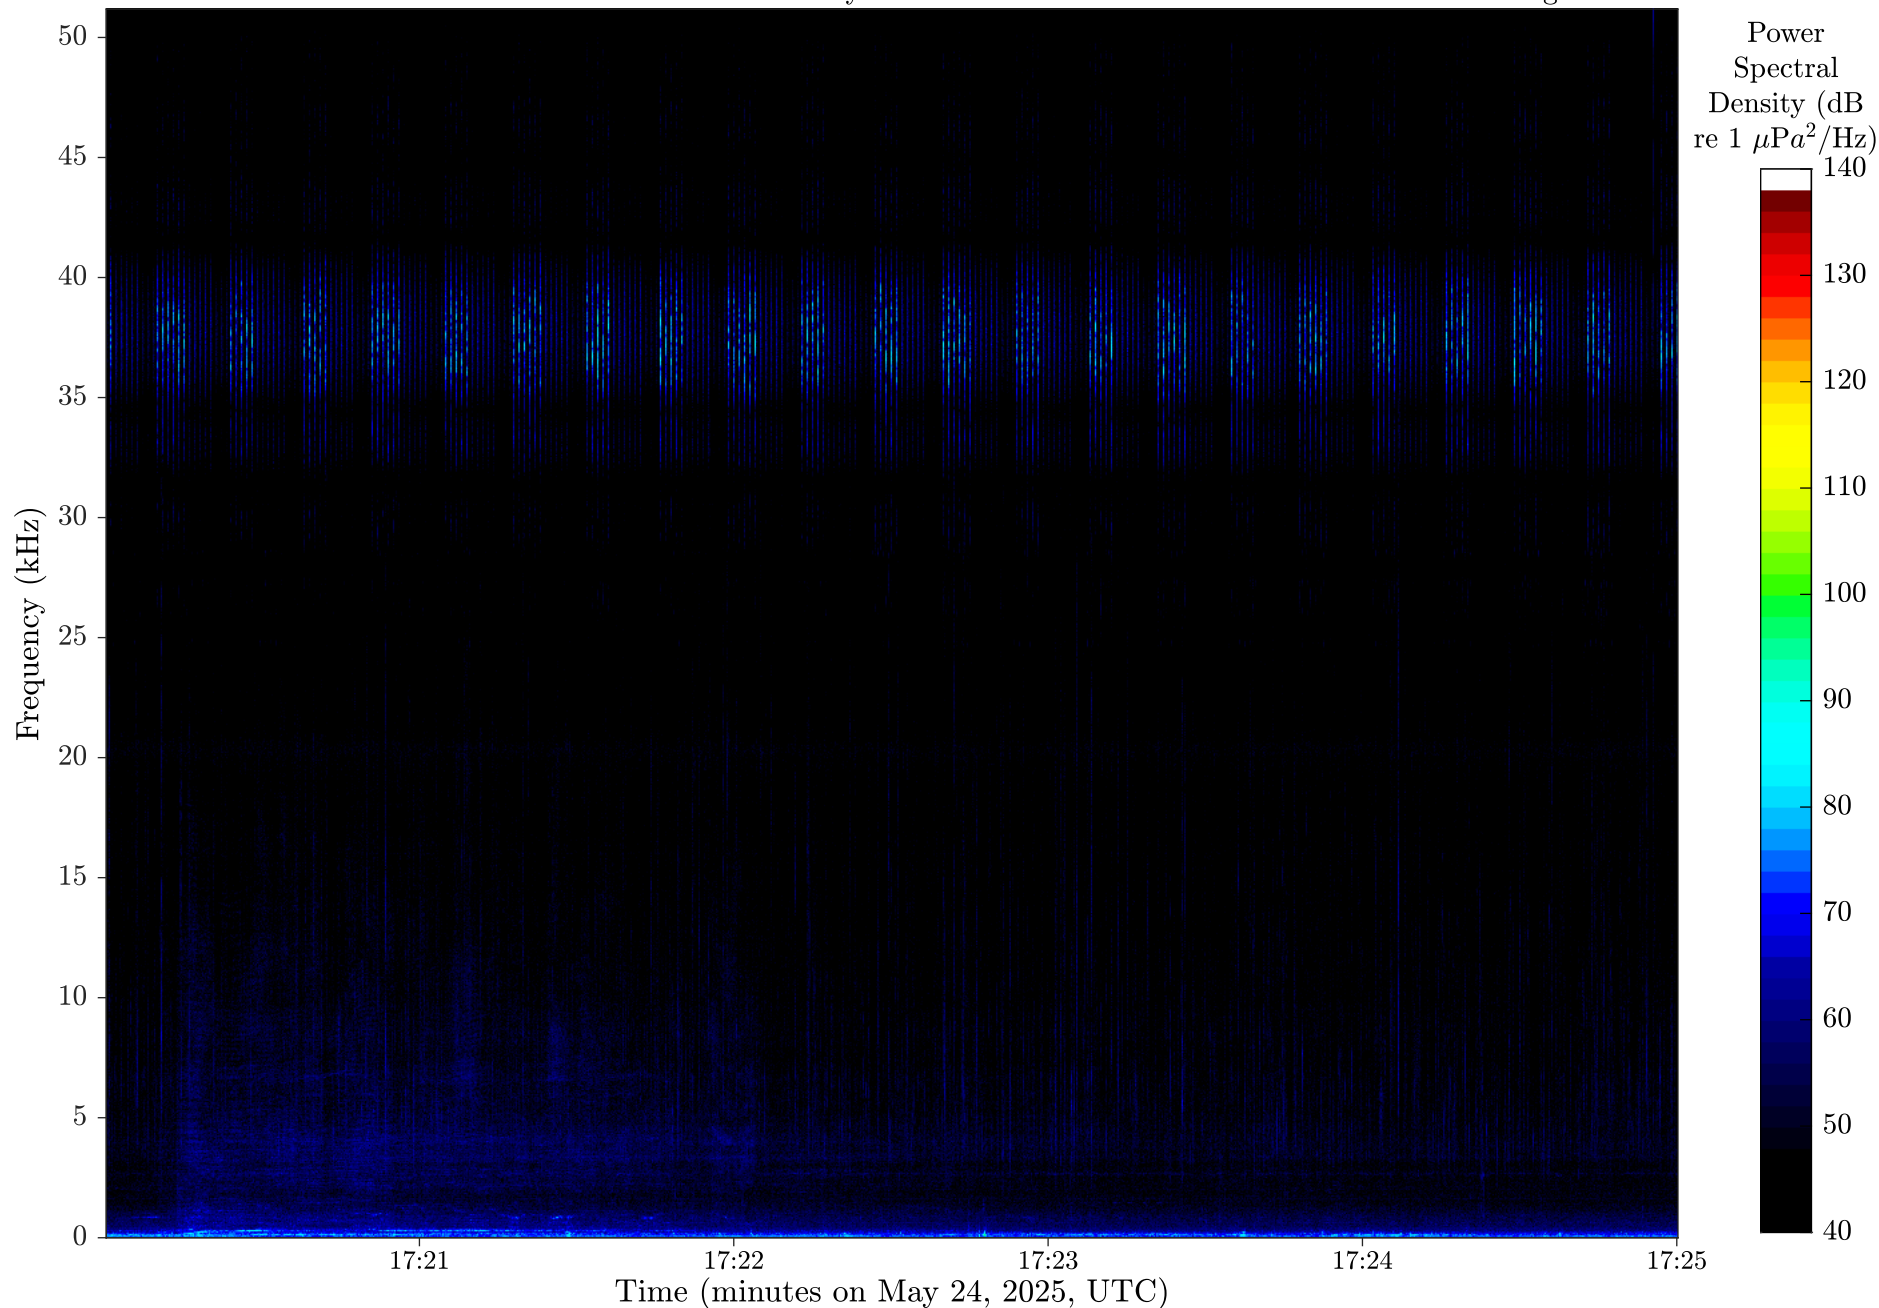

Comments: 32.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:43:56 UTC

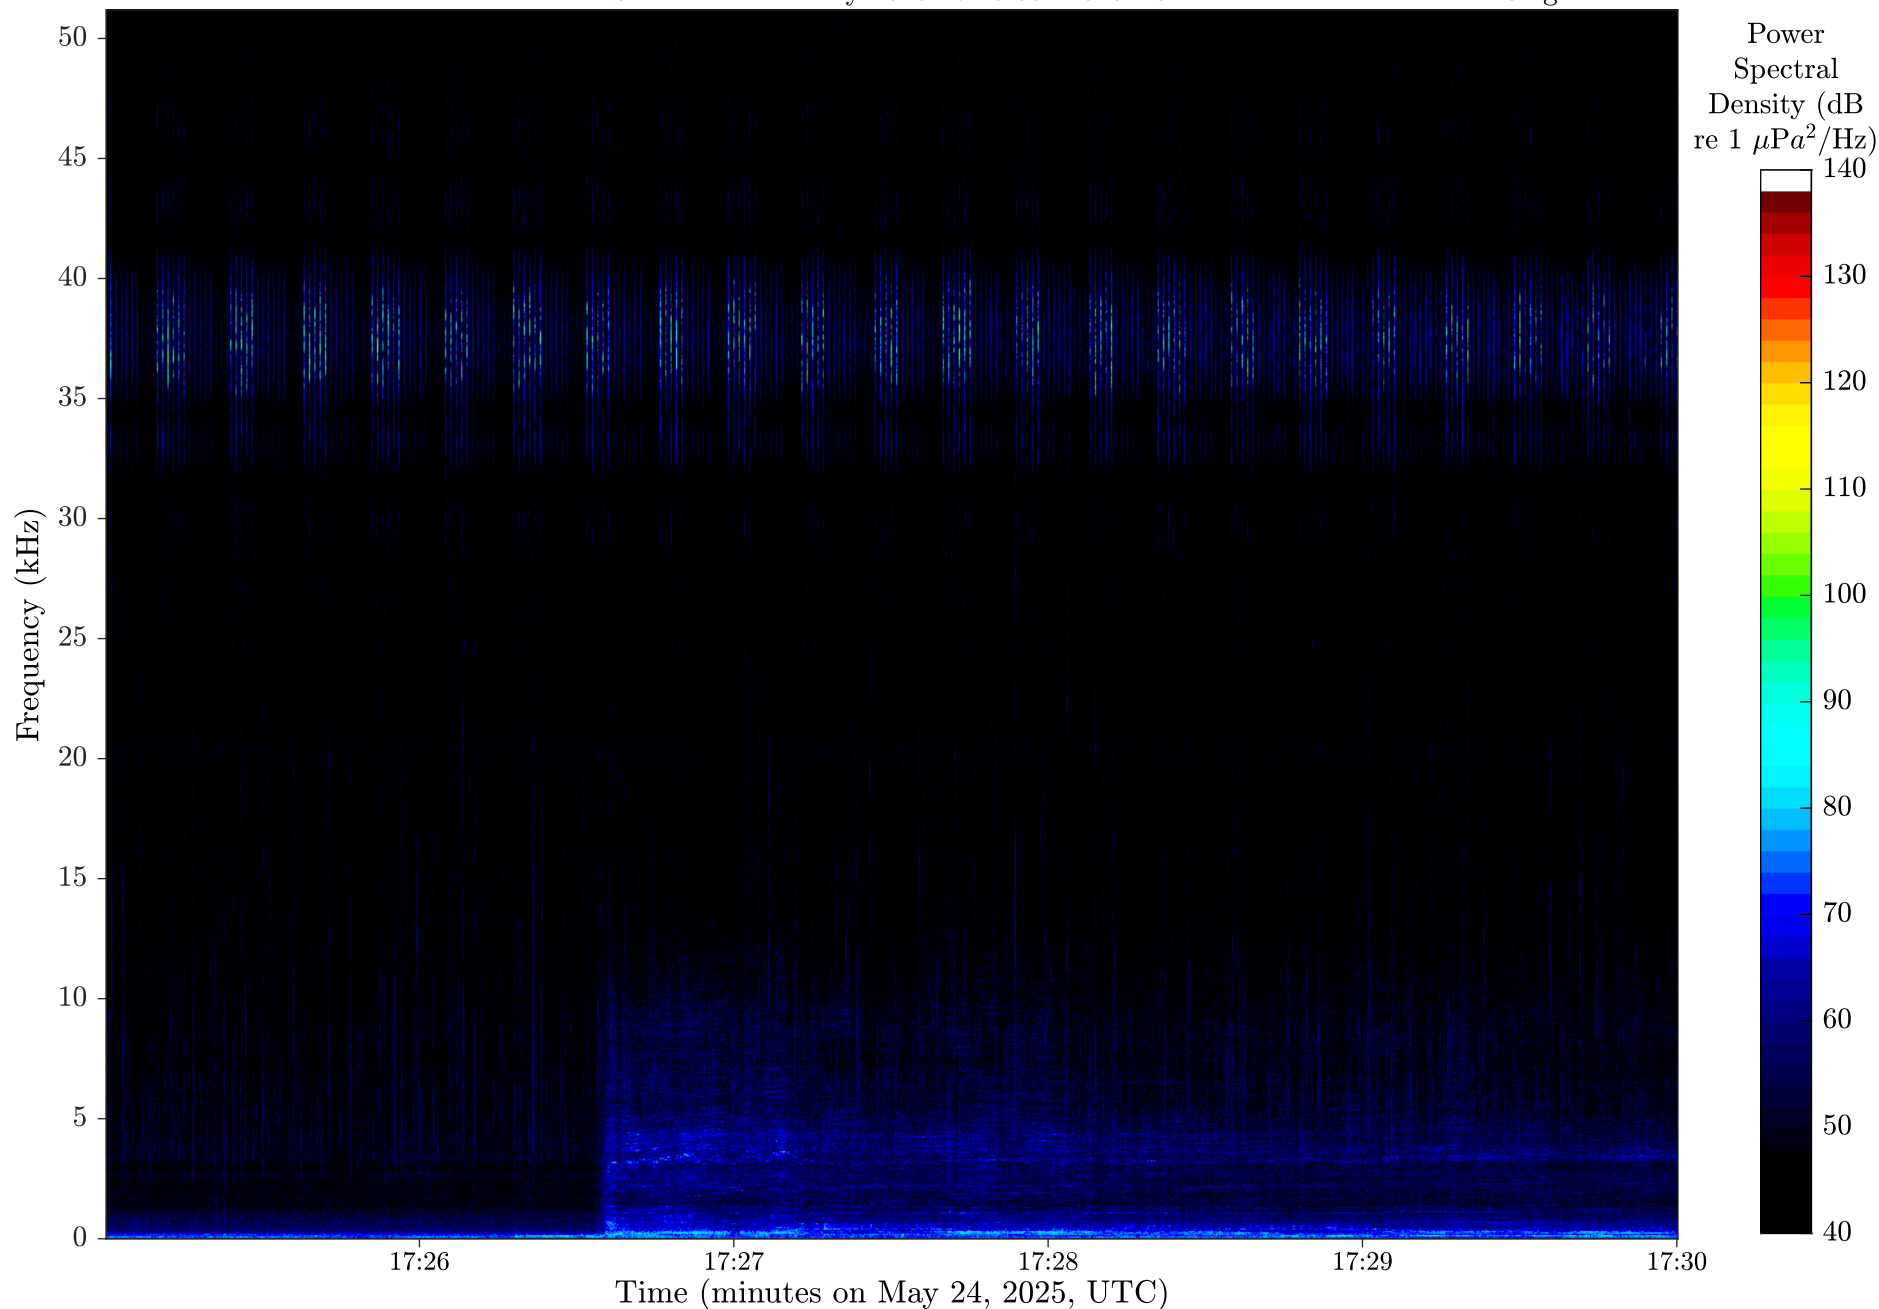

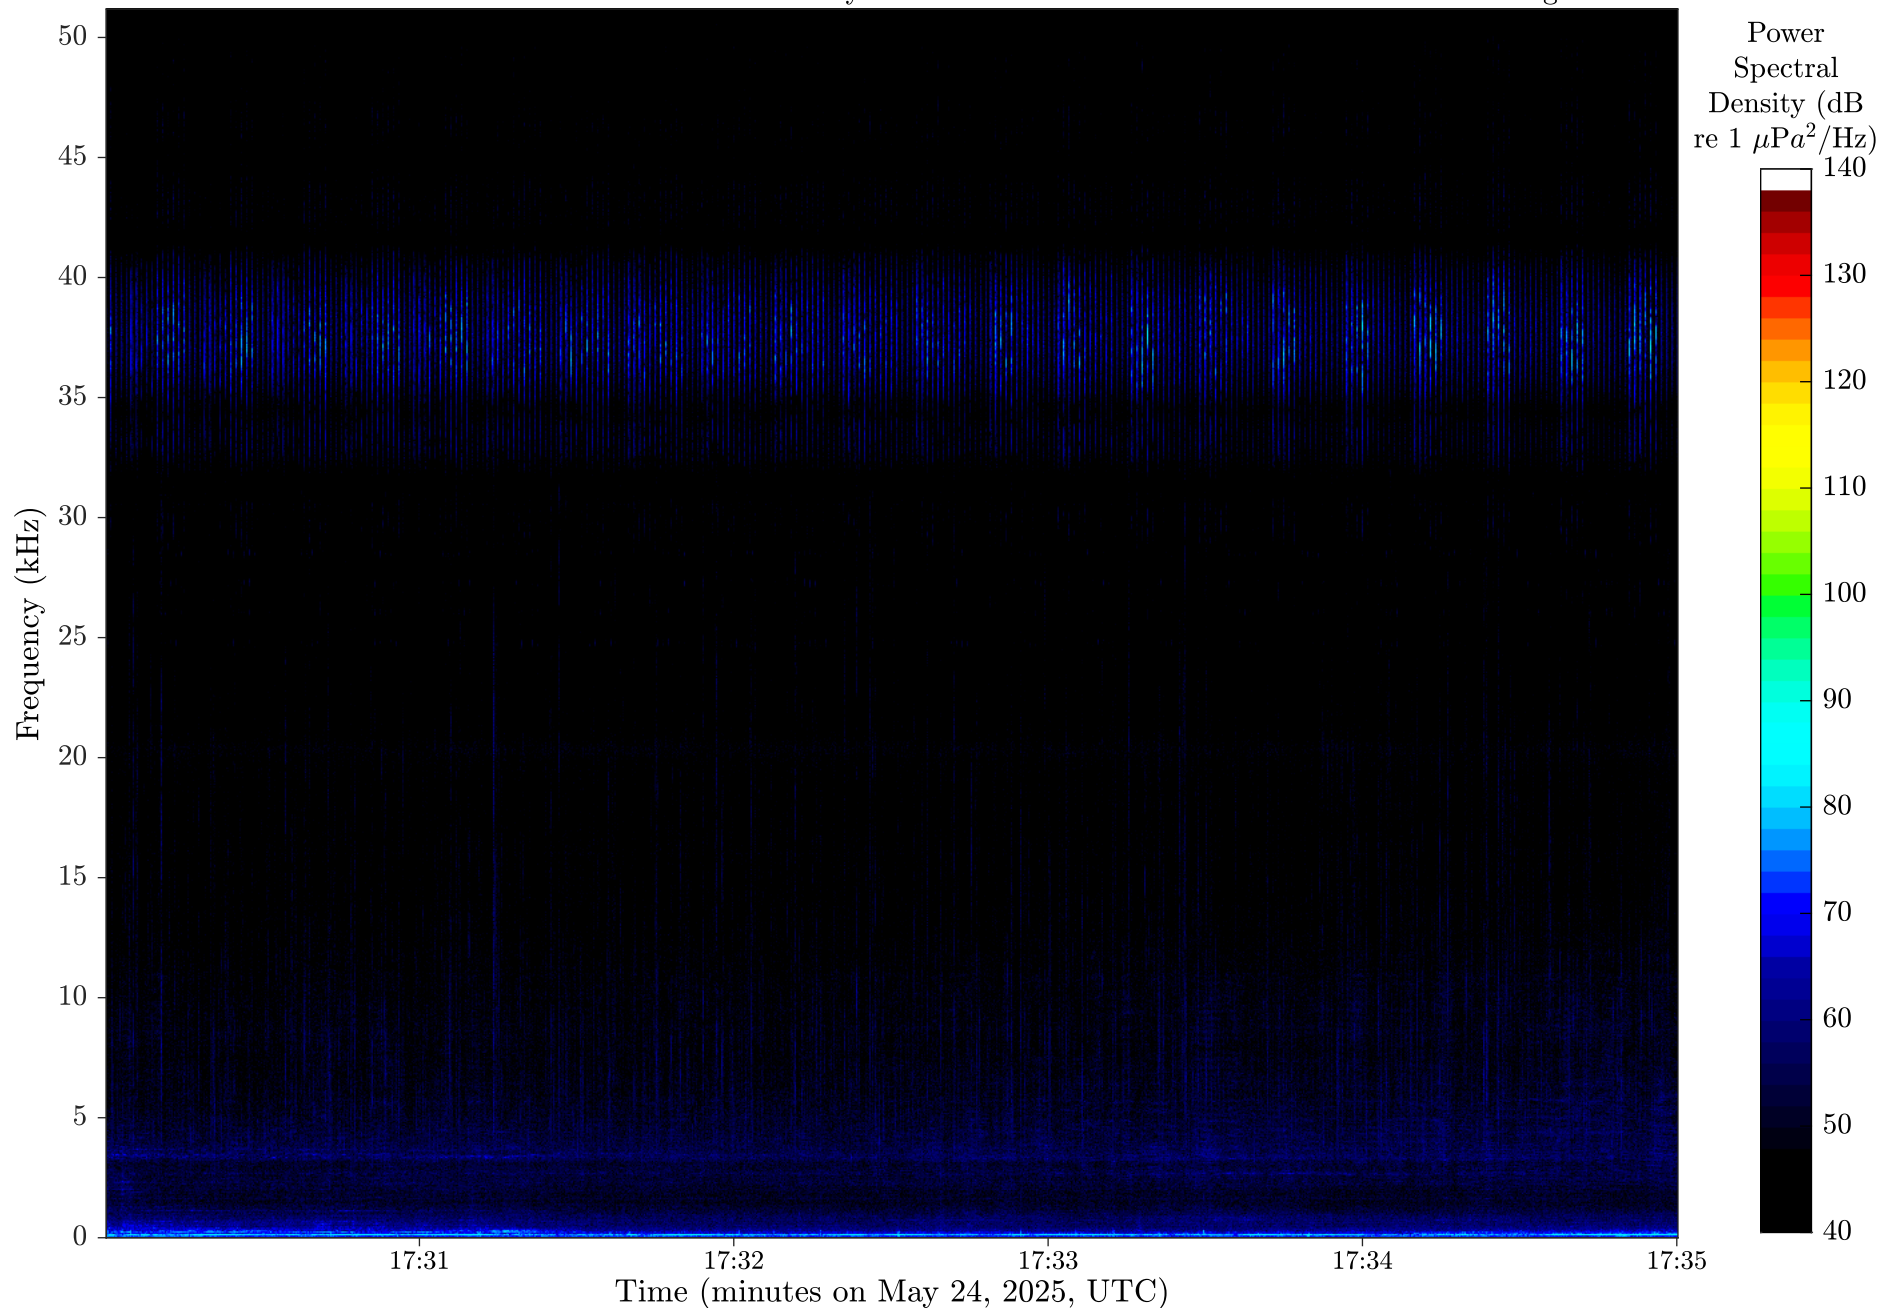


Comments: 31.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:12 UTC

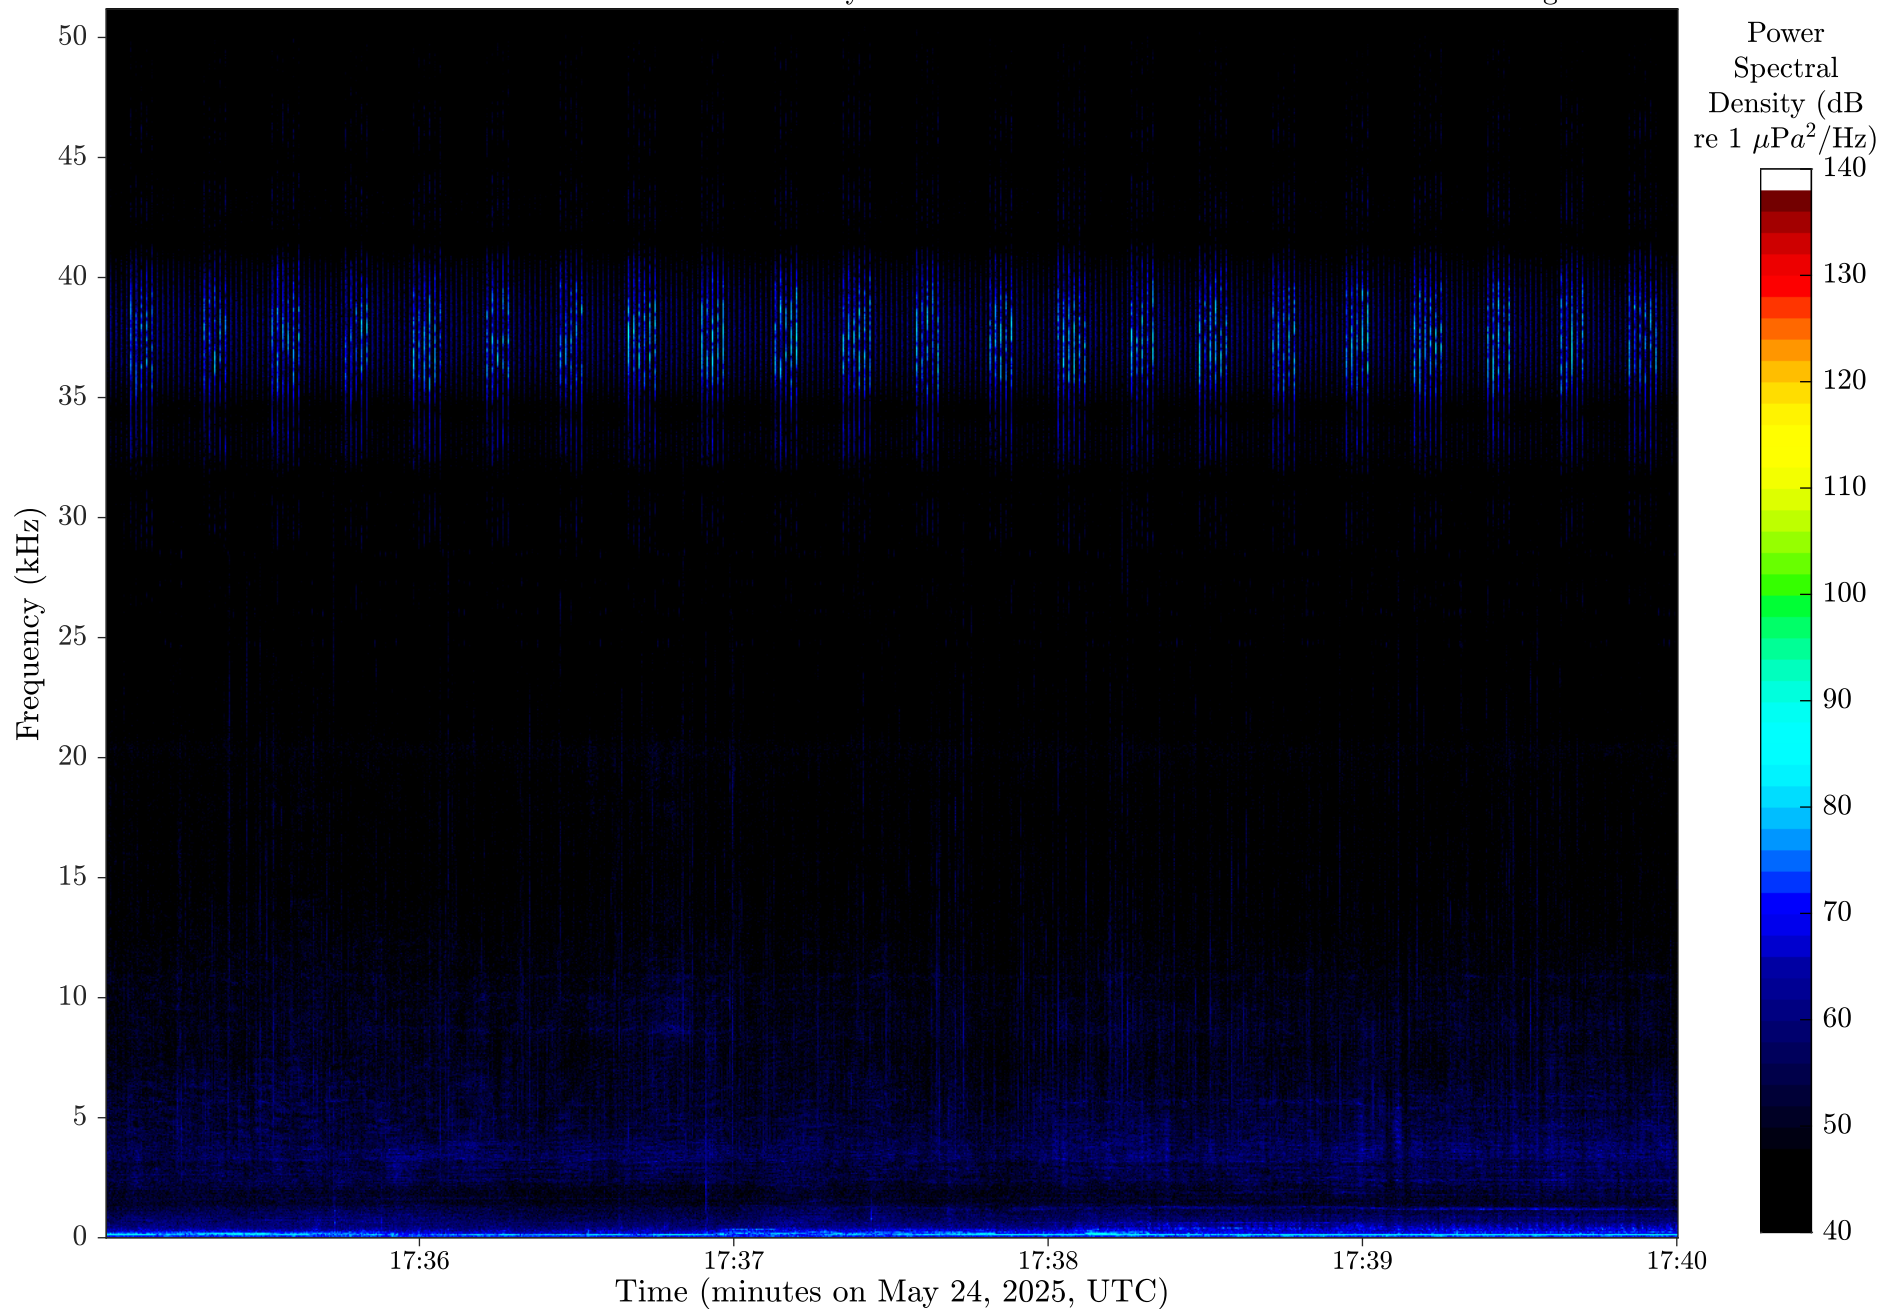


Comments: 30.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:20 UTC

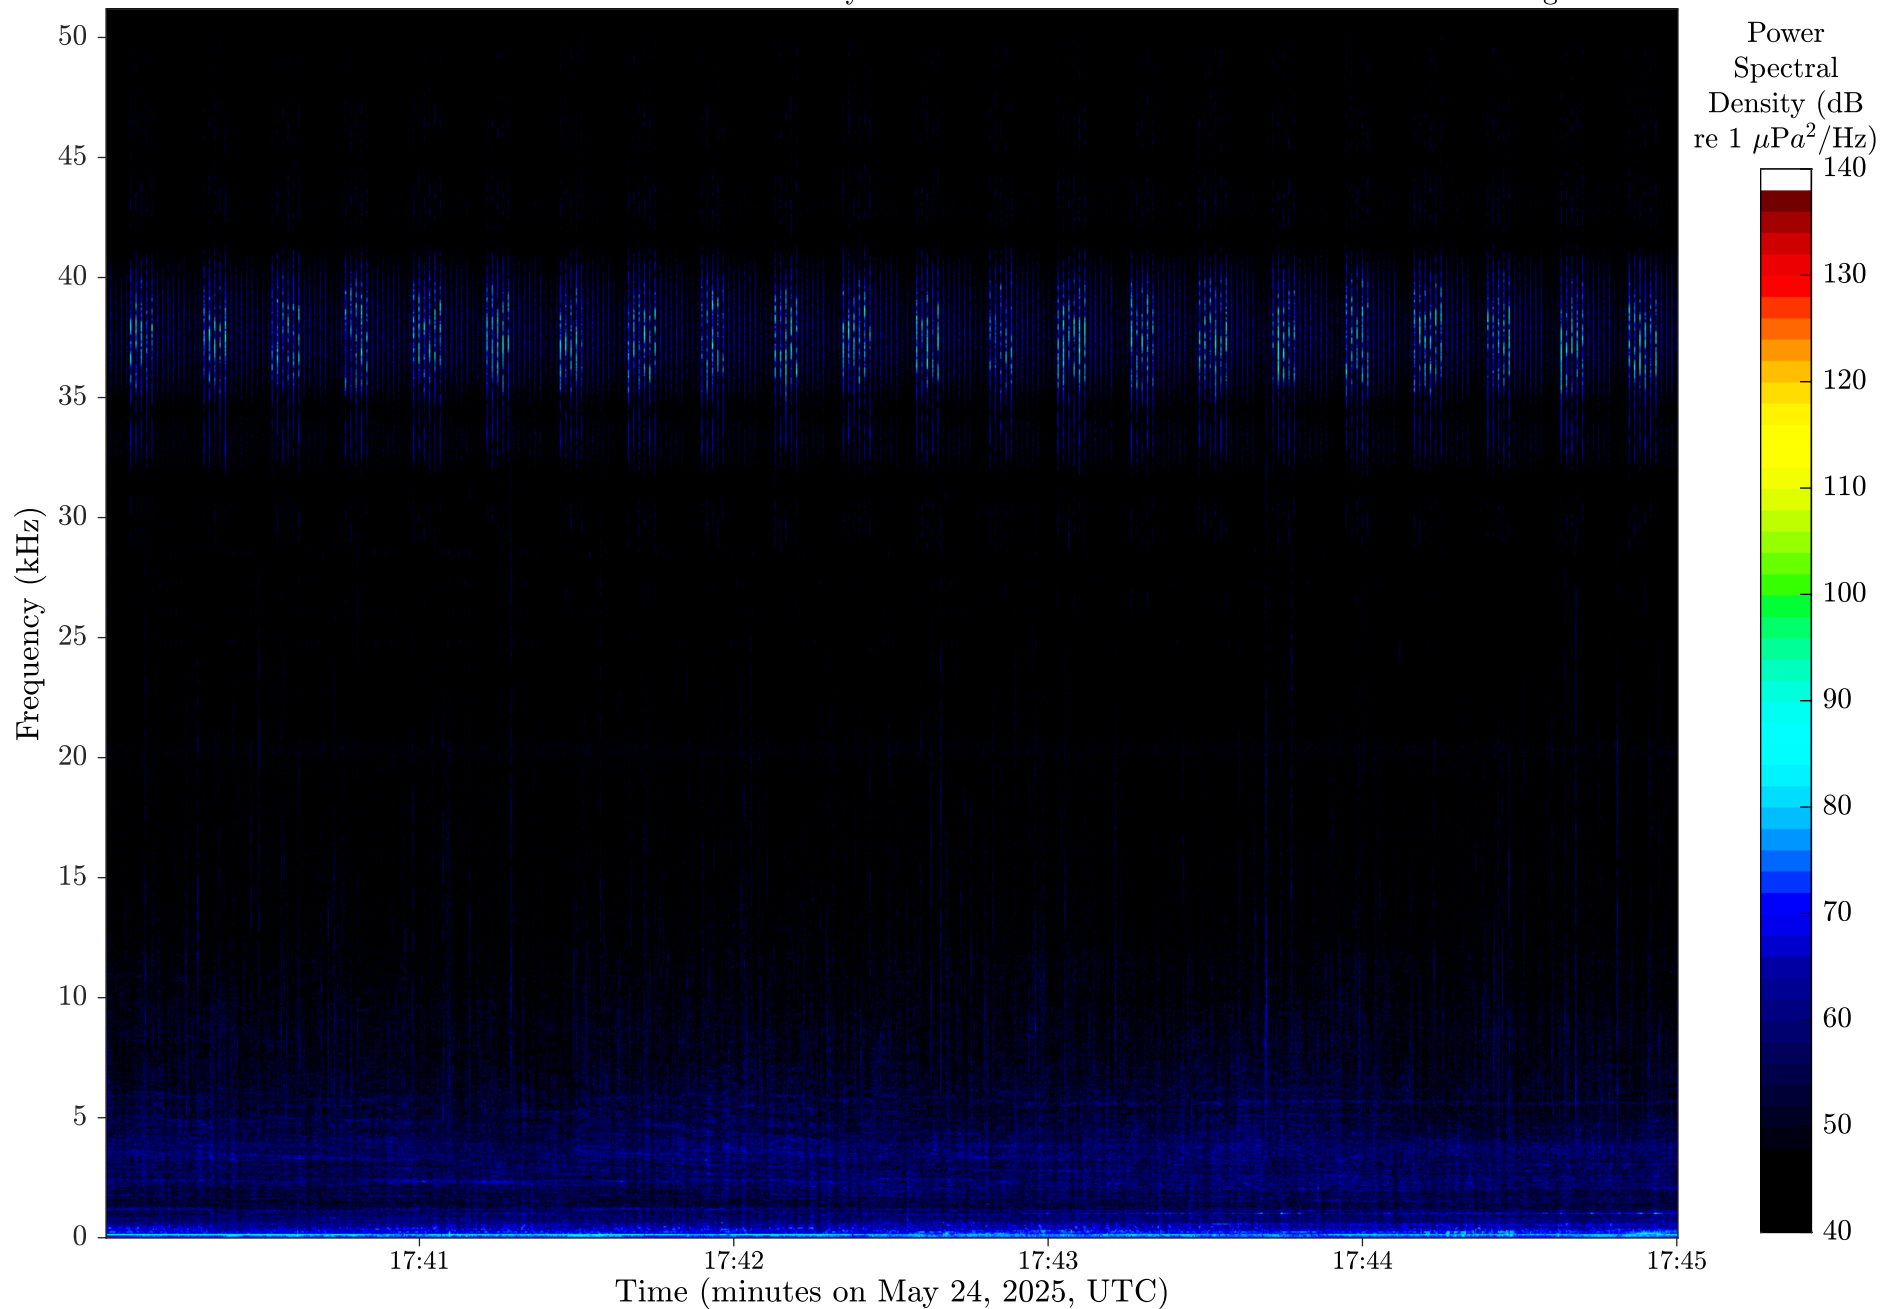


Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:28 UTC

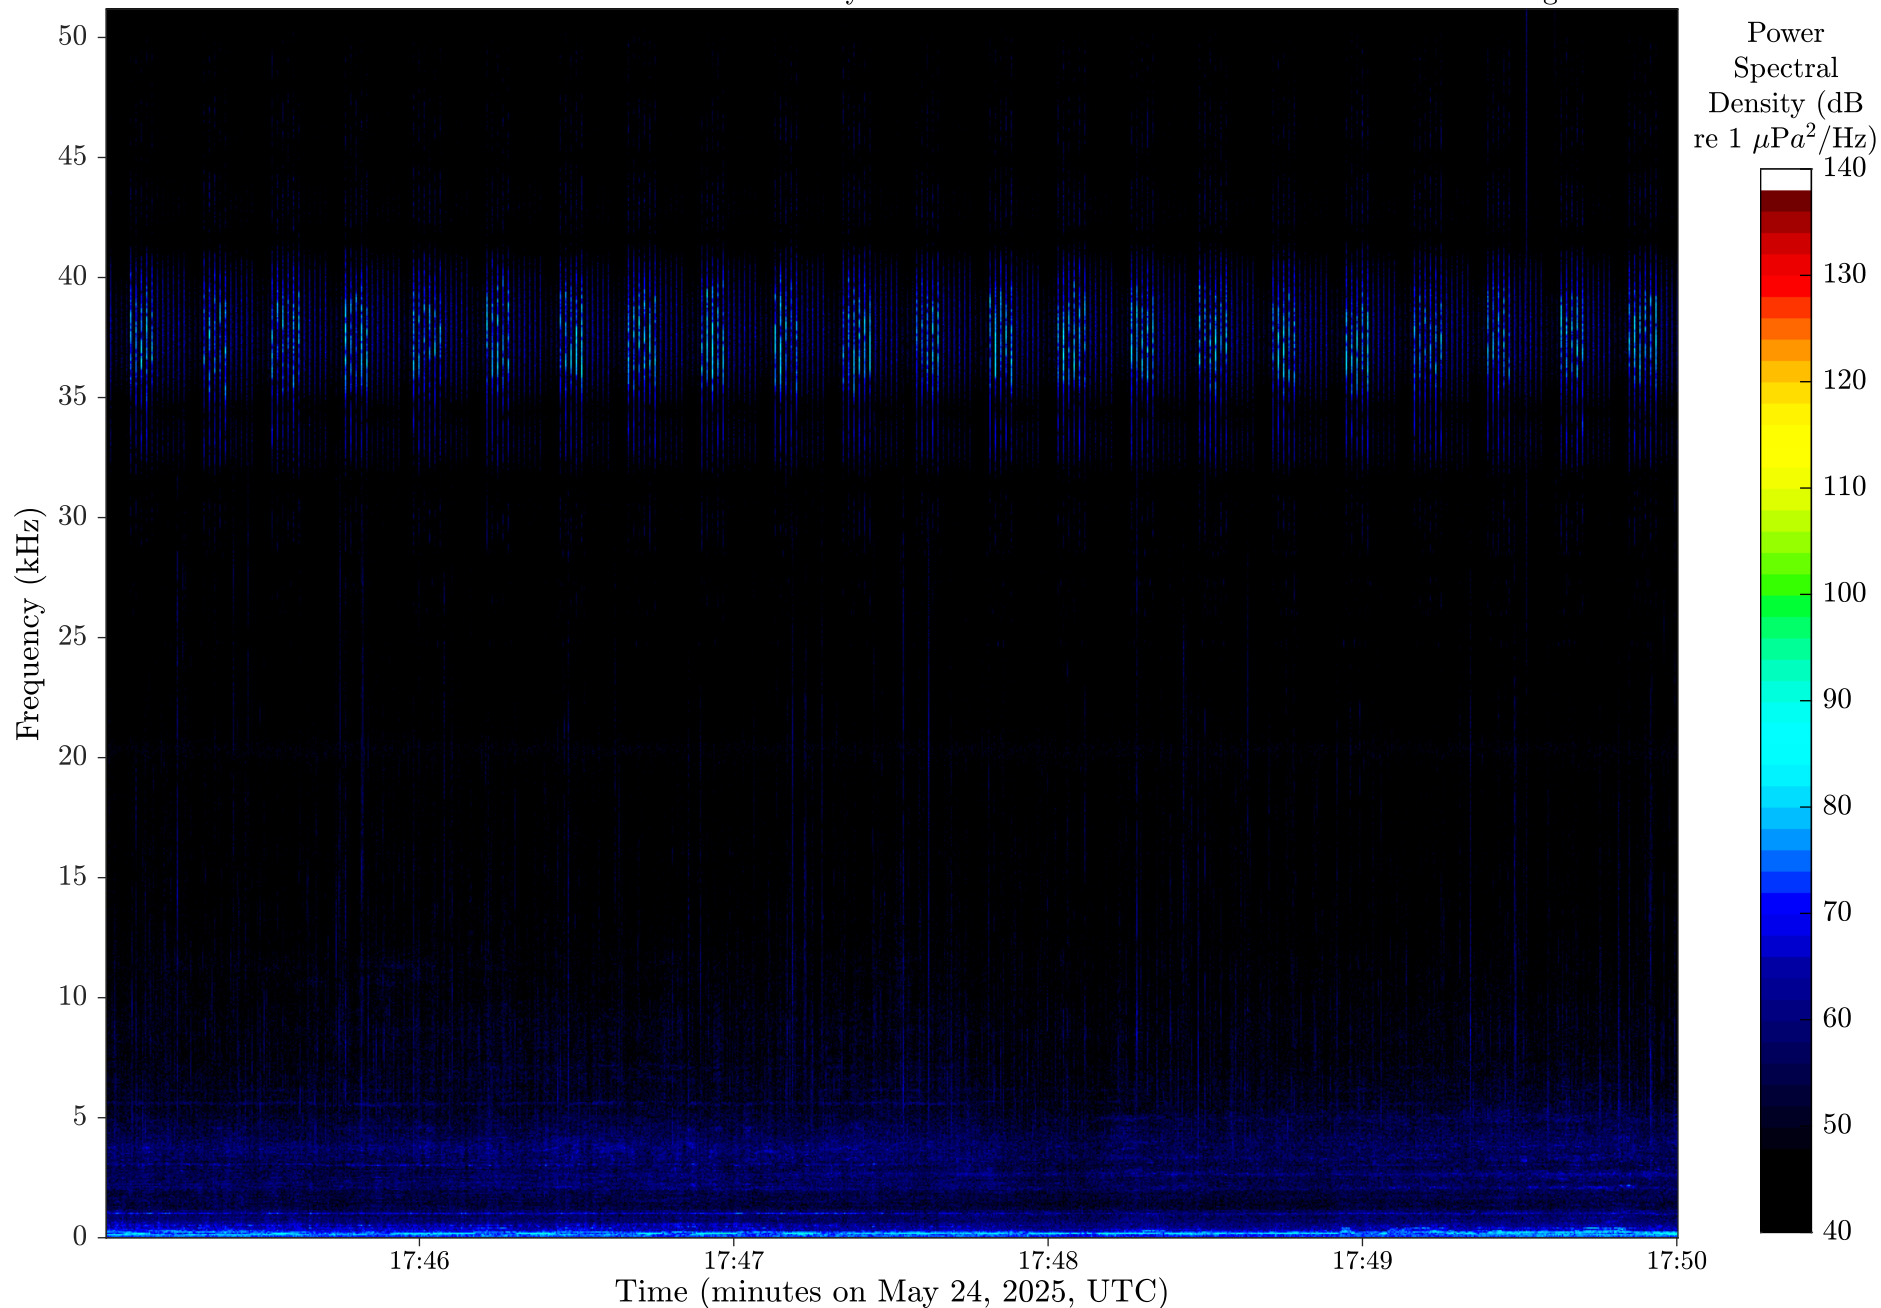


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:36 UTC

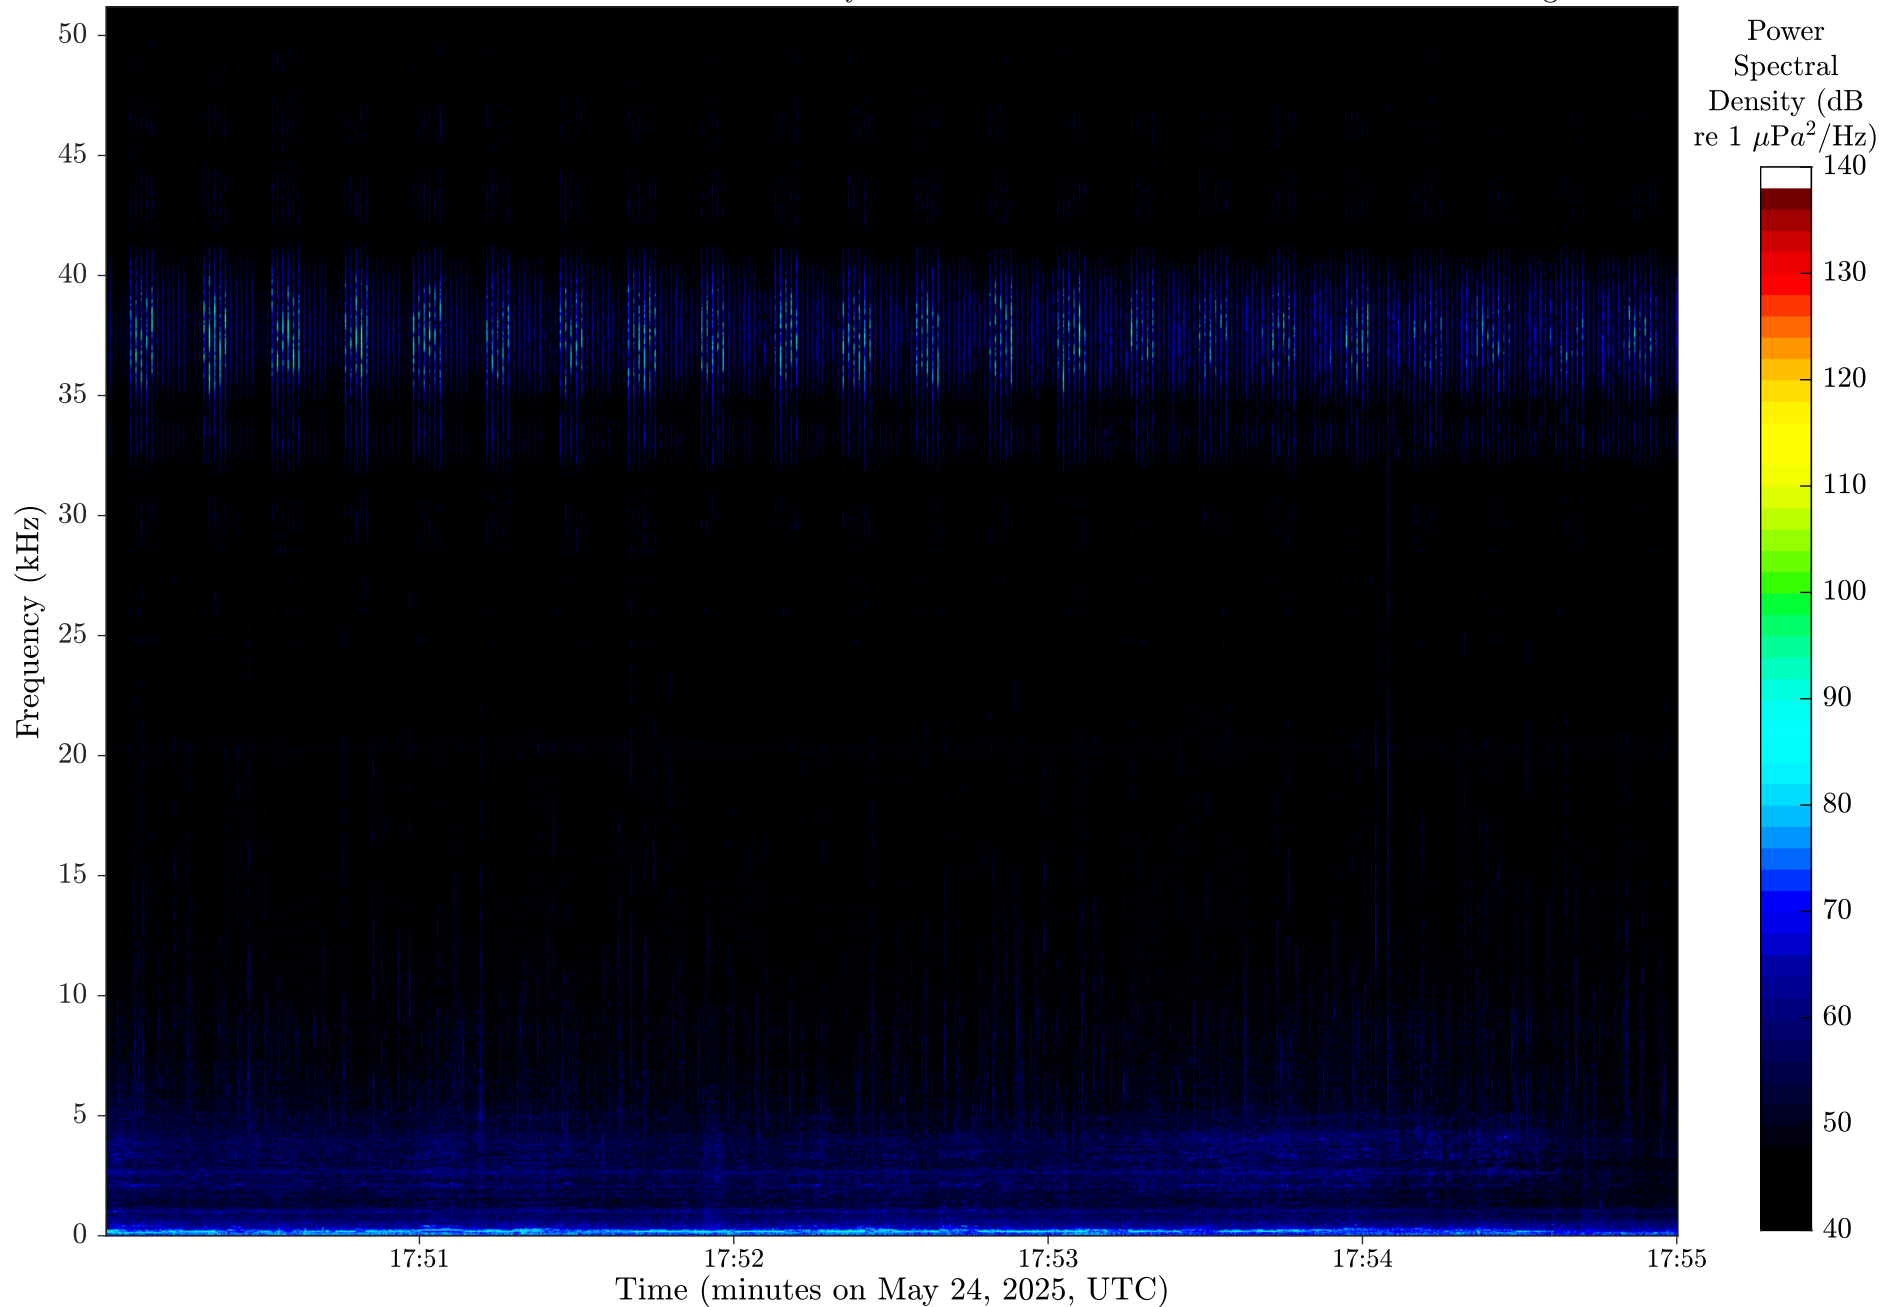


Comments: 32.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:44 UTC

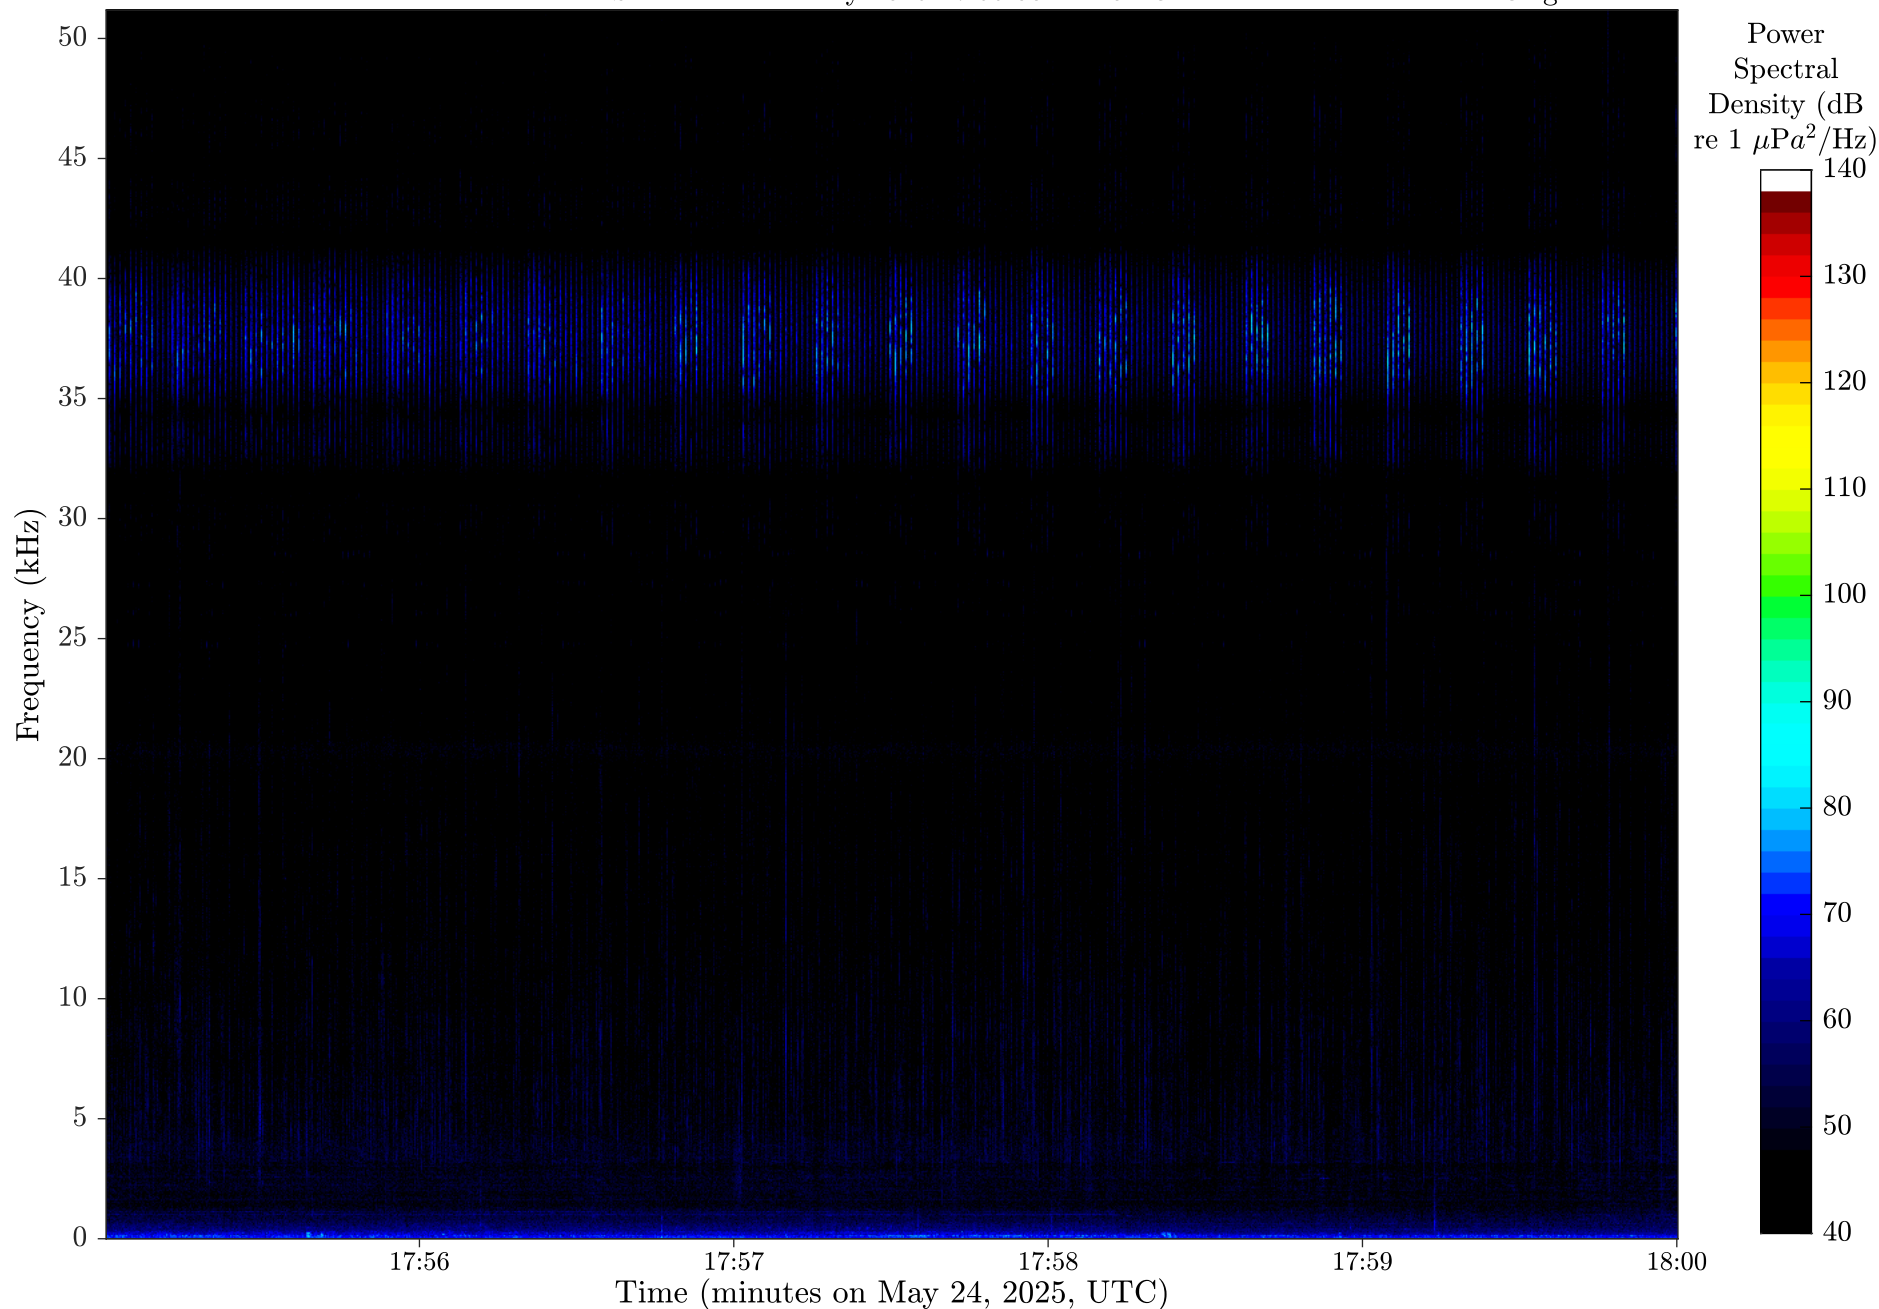


Comments: 32.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:53 UTC

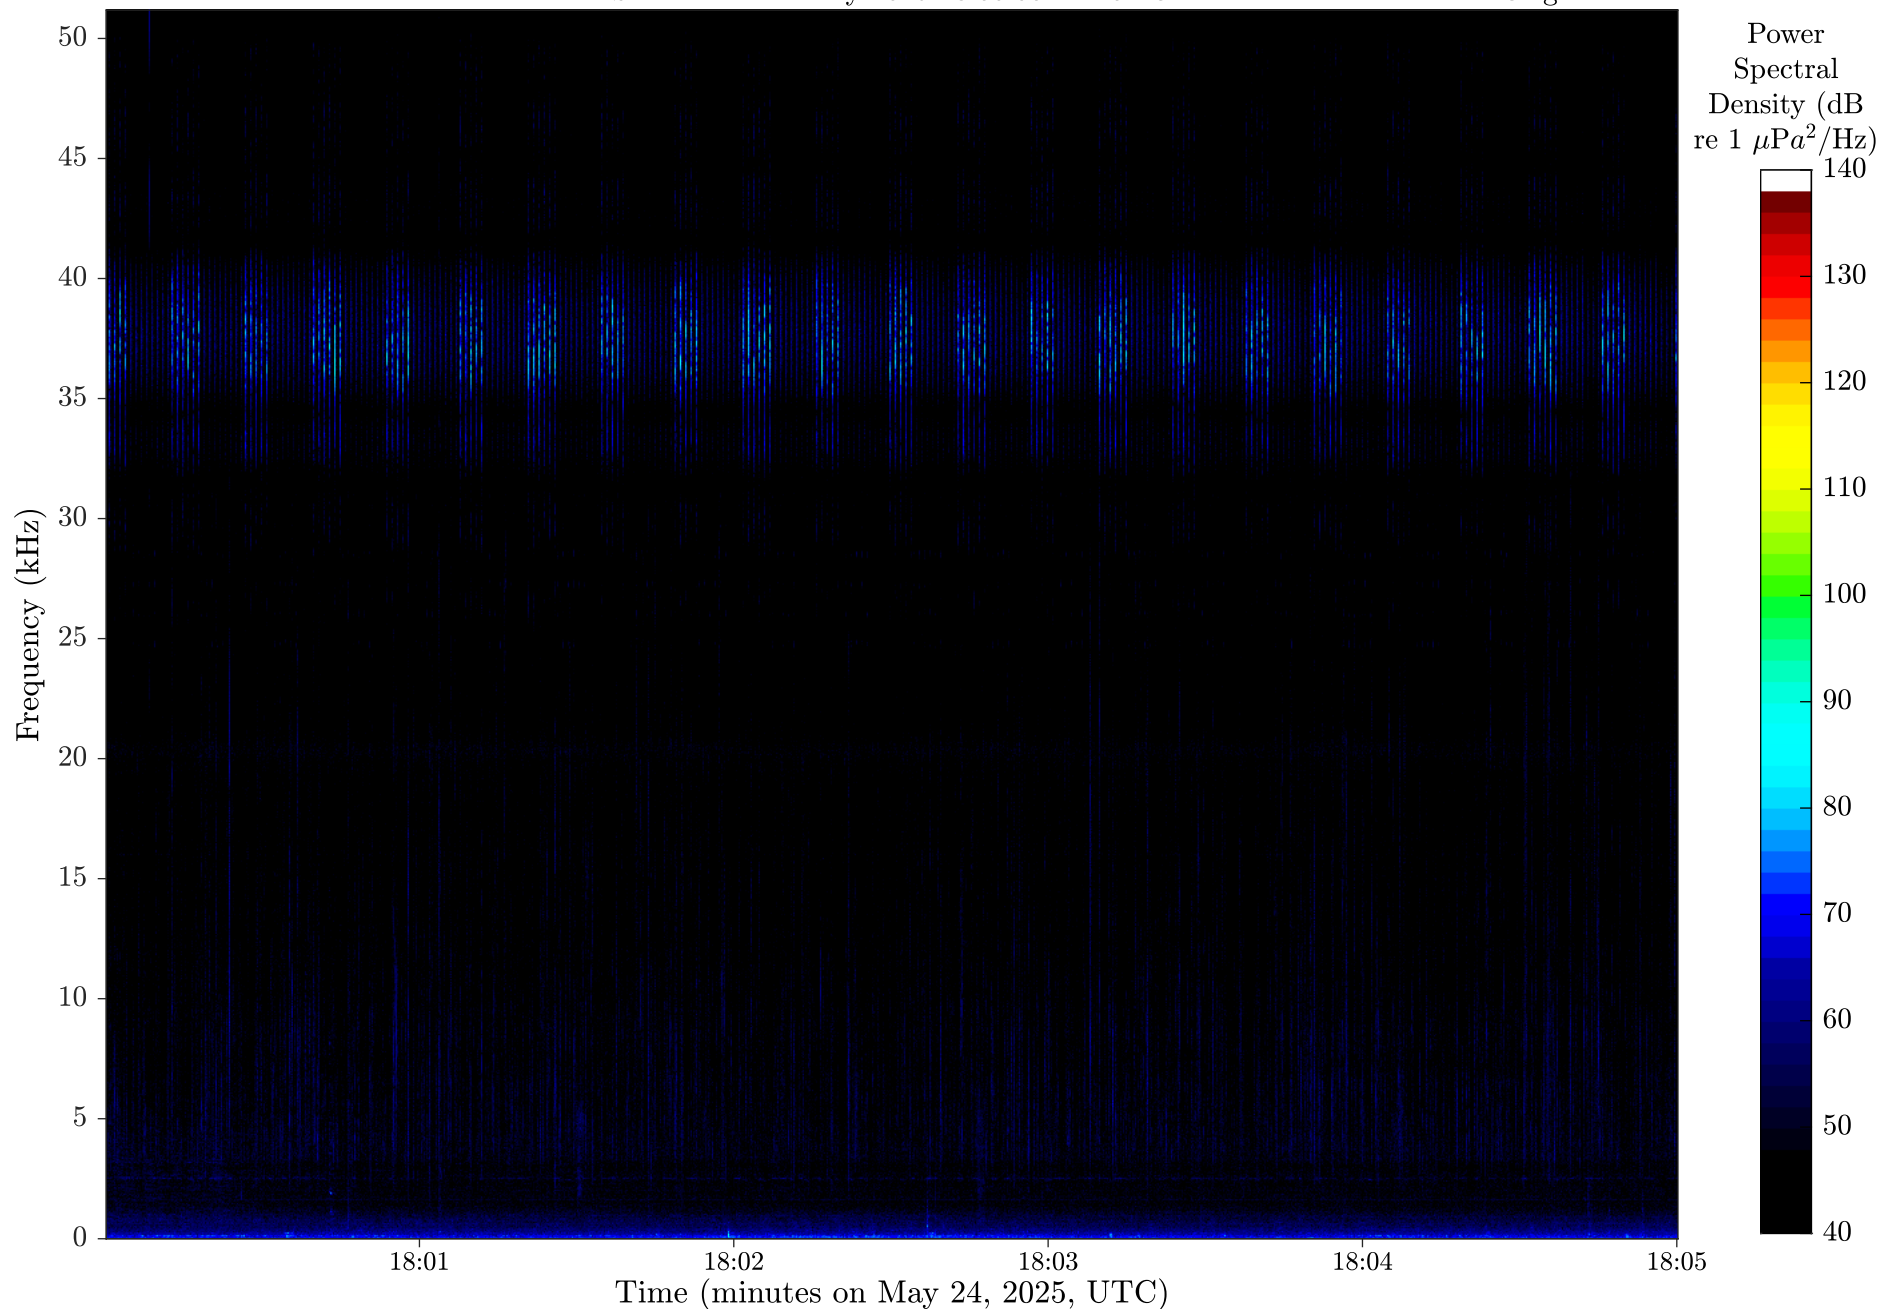


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:45:01 UTC

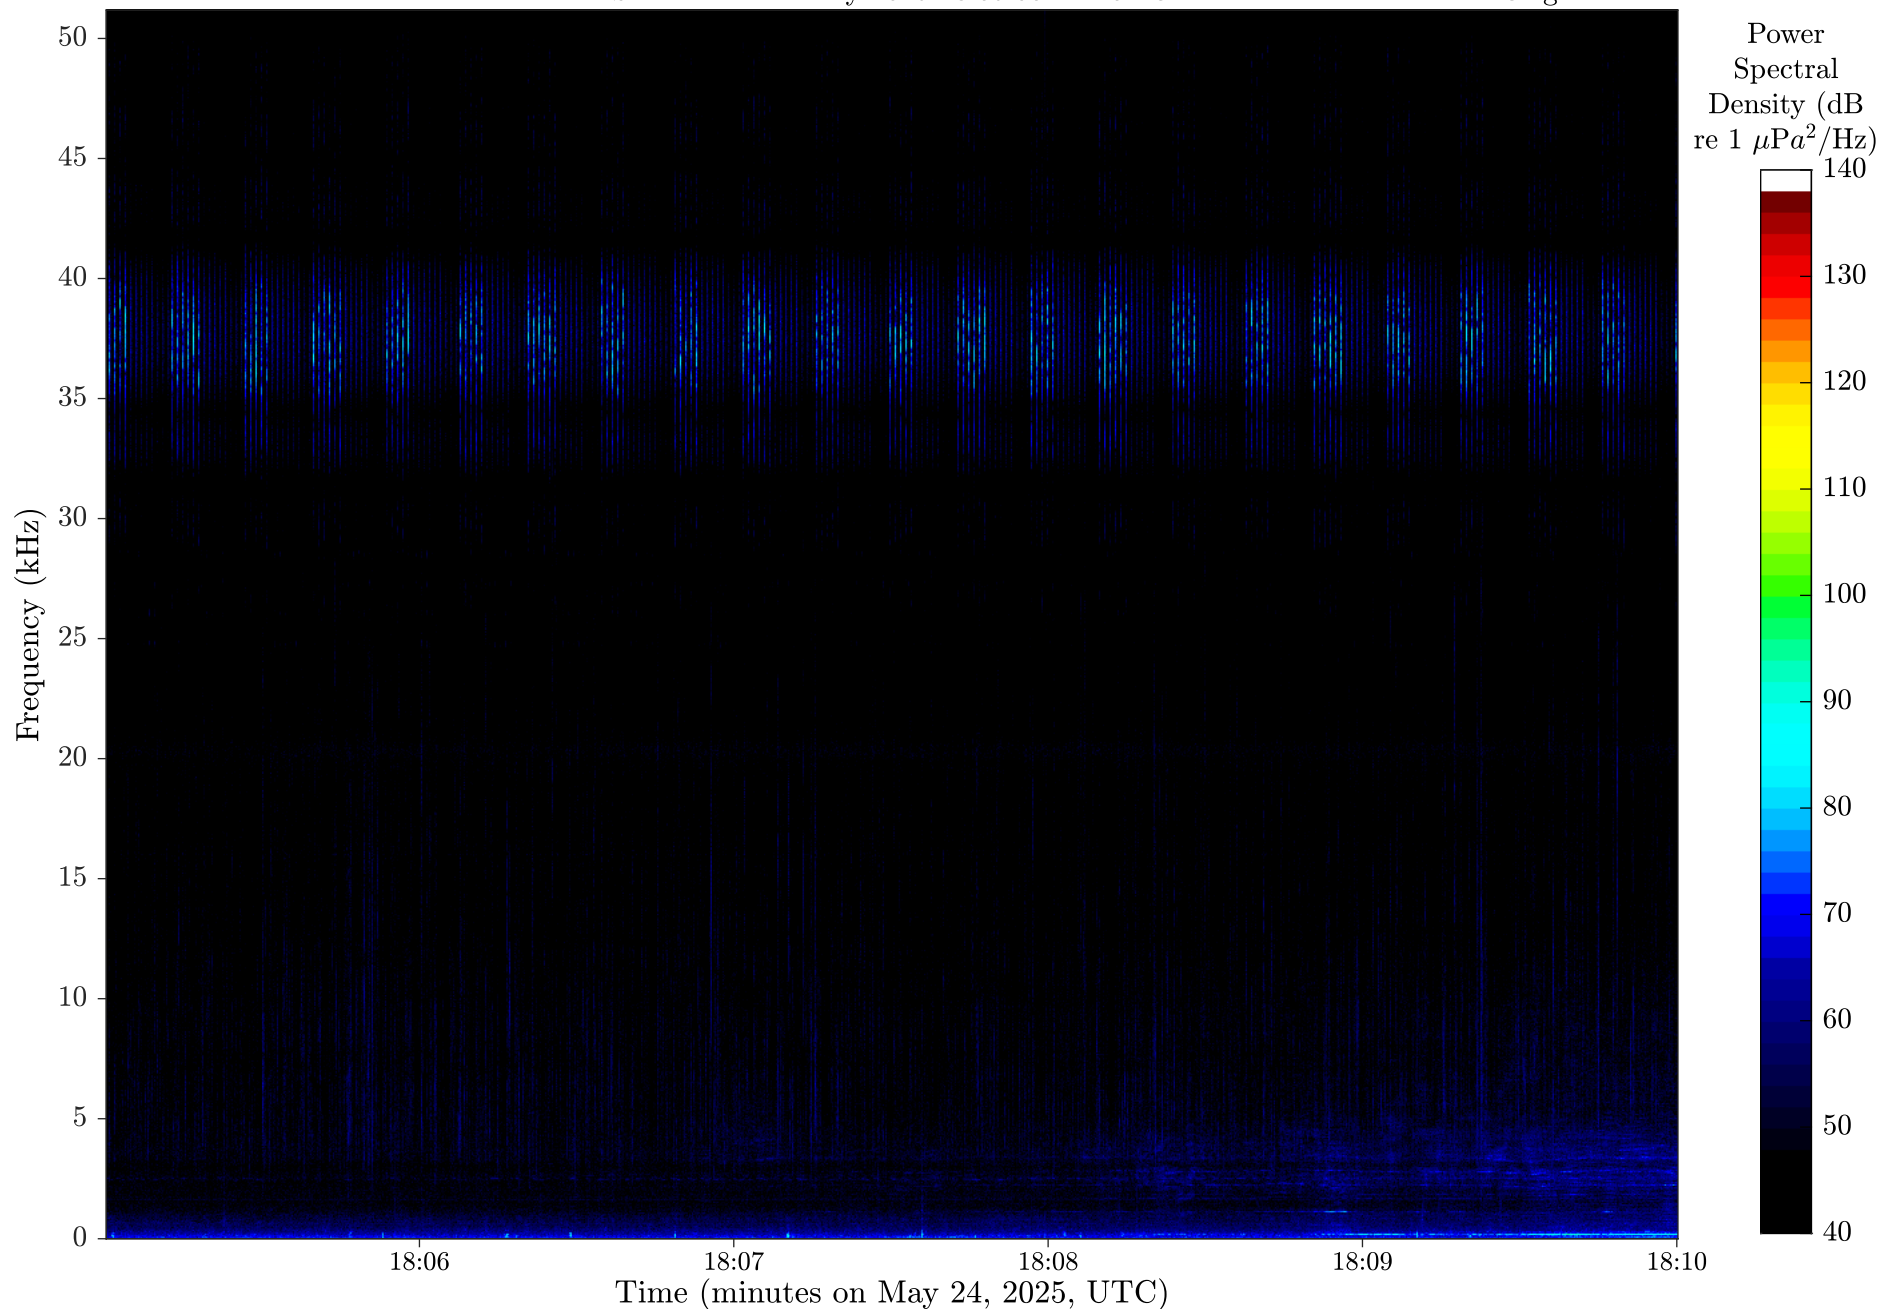

Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:45:09 UTC

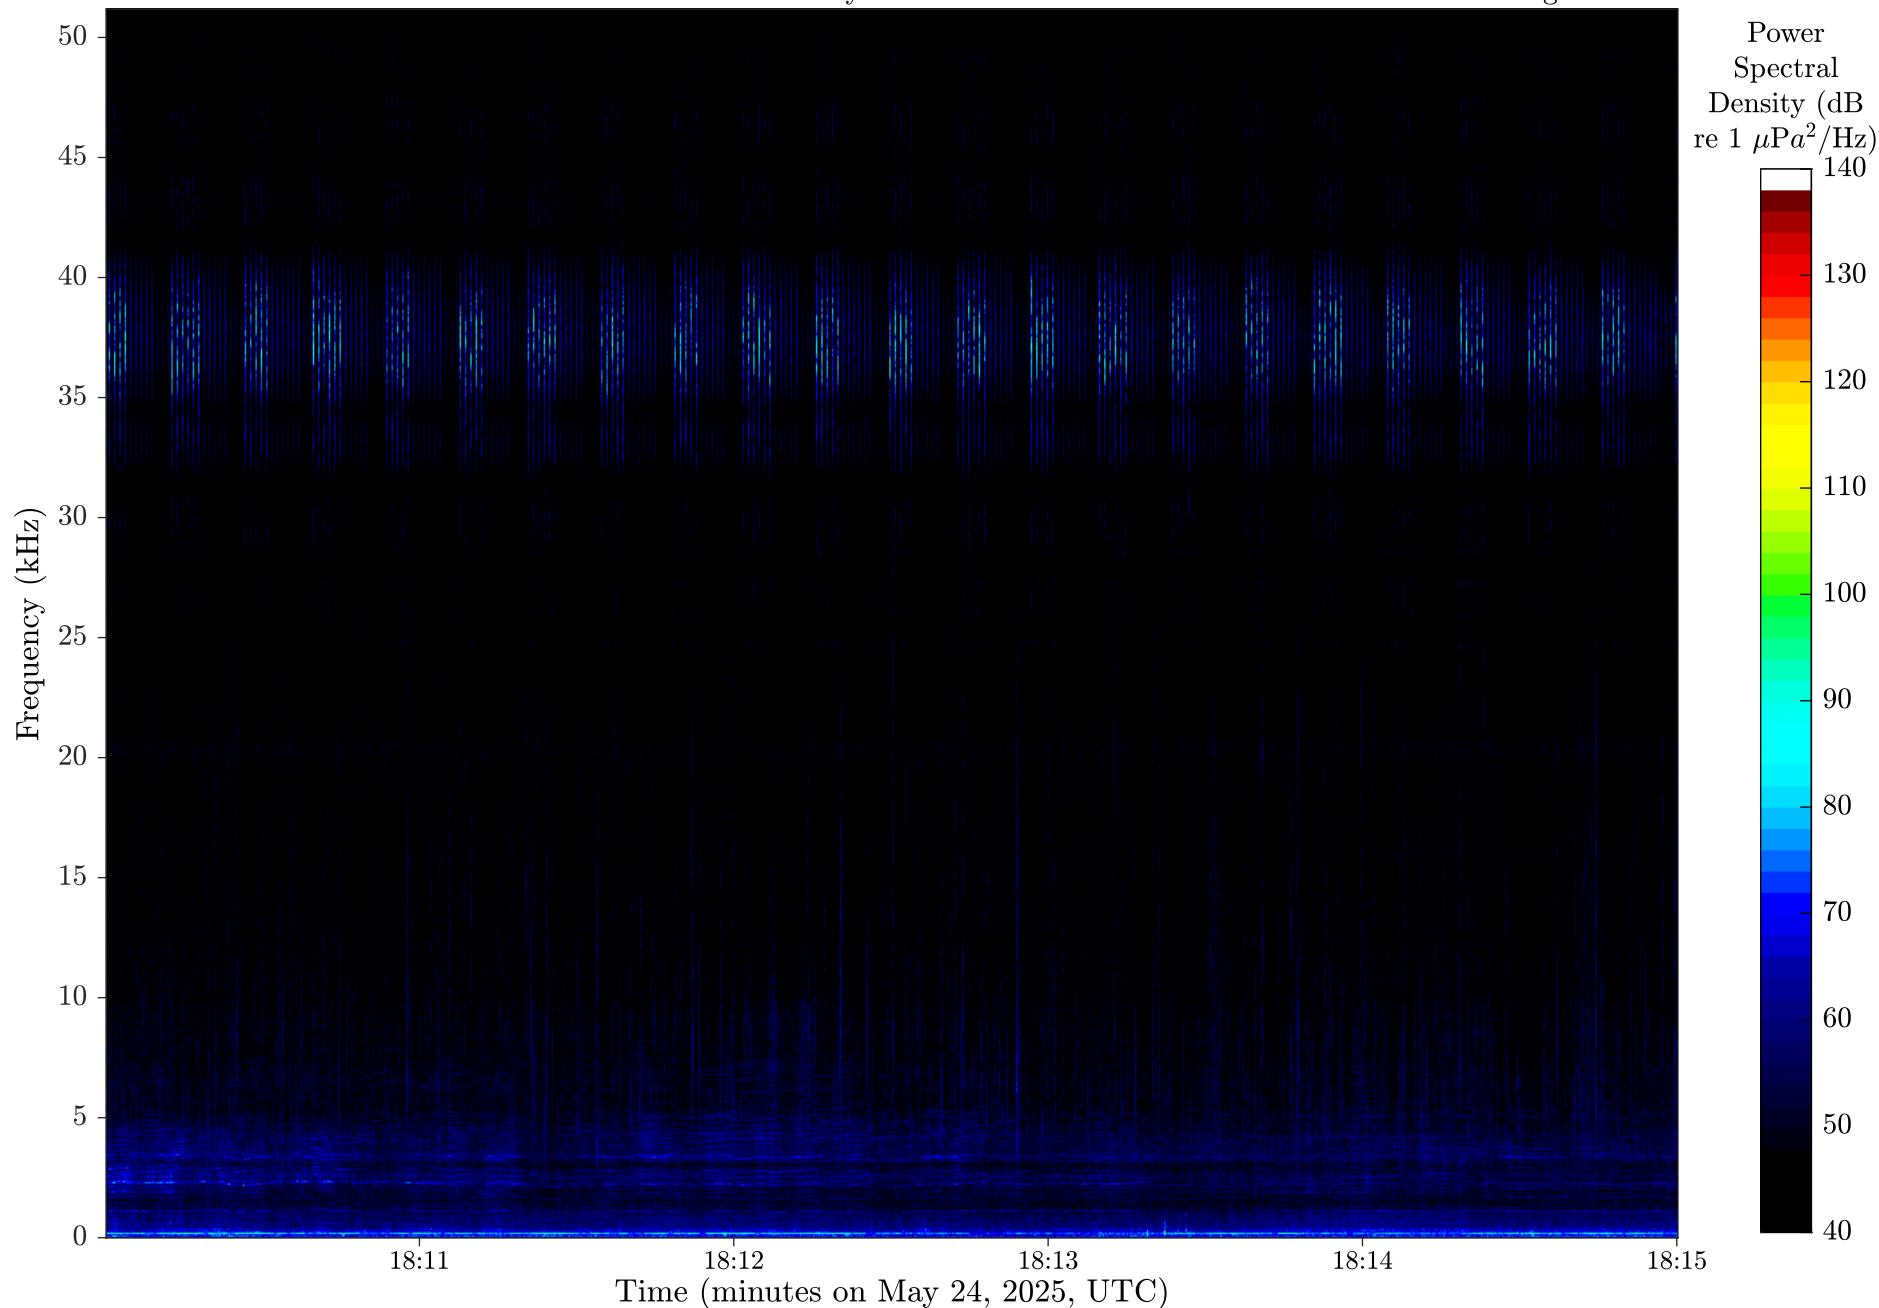


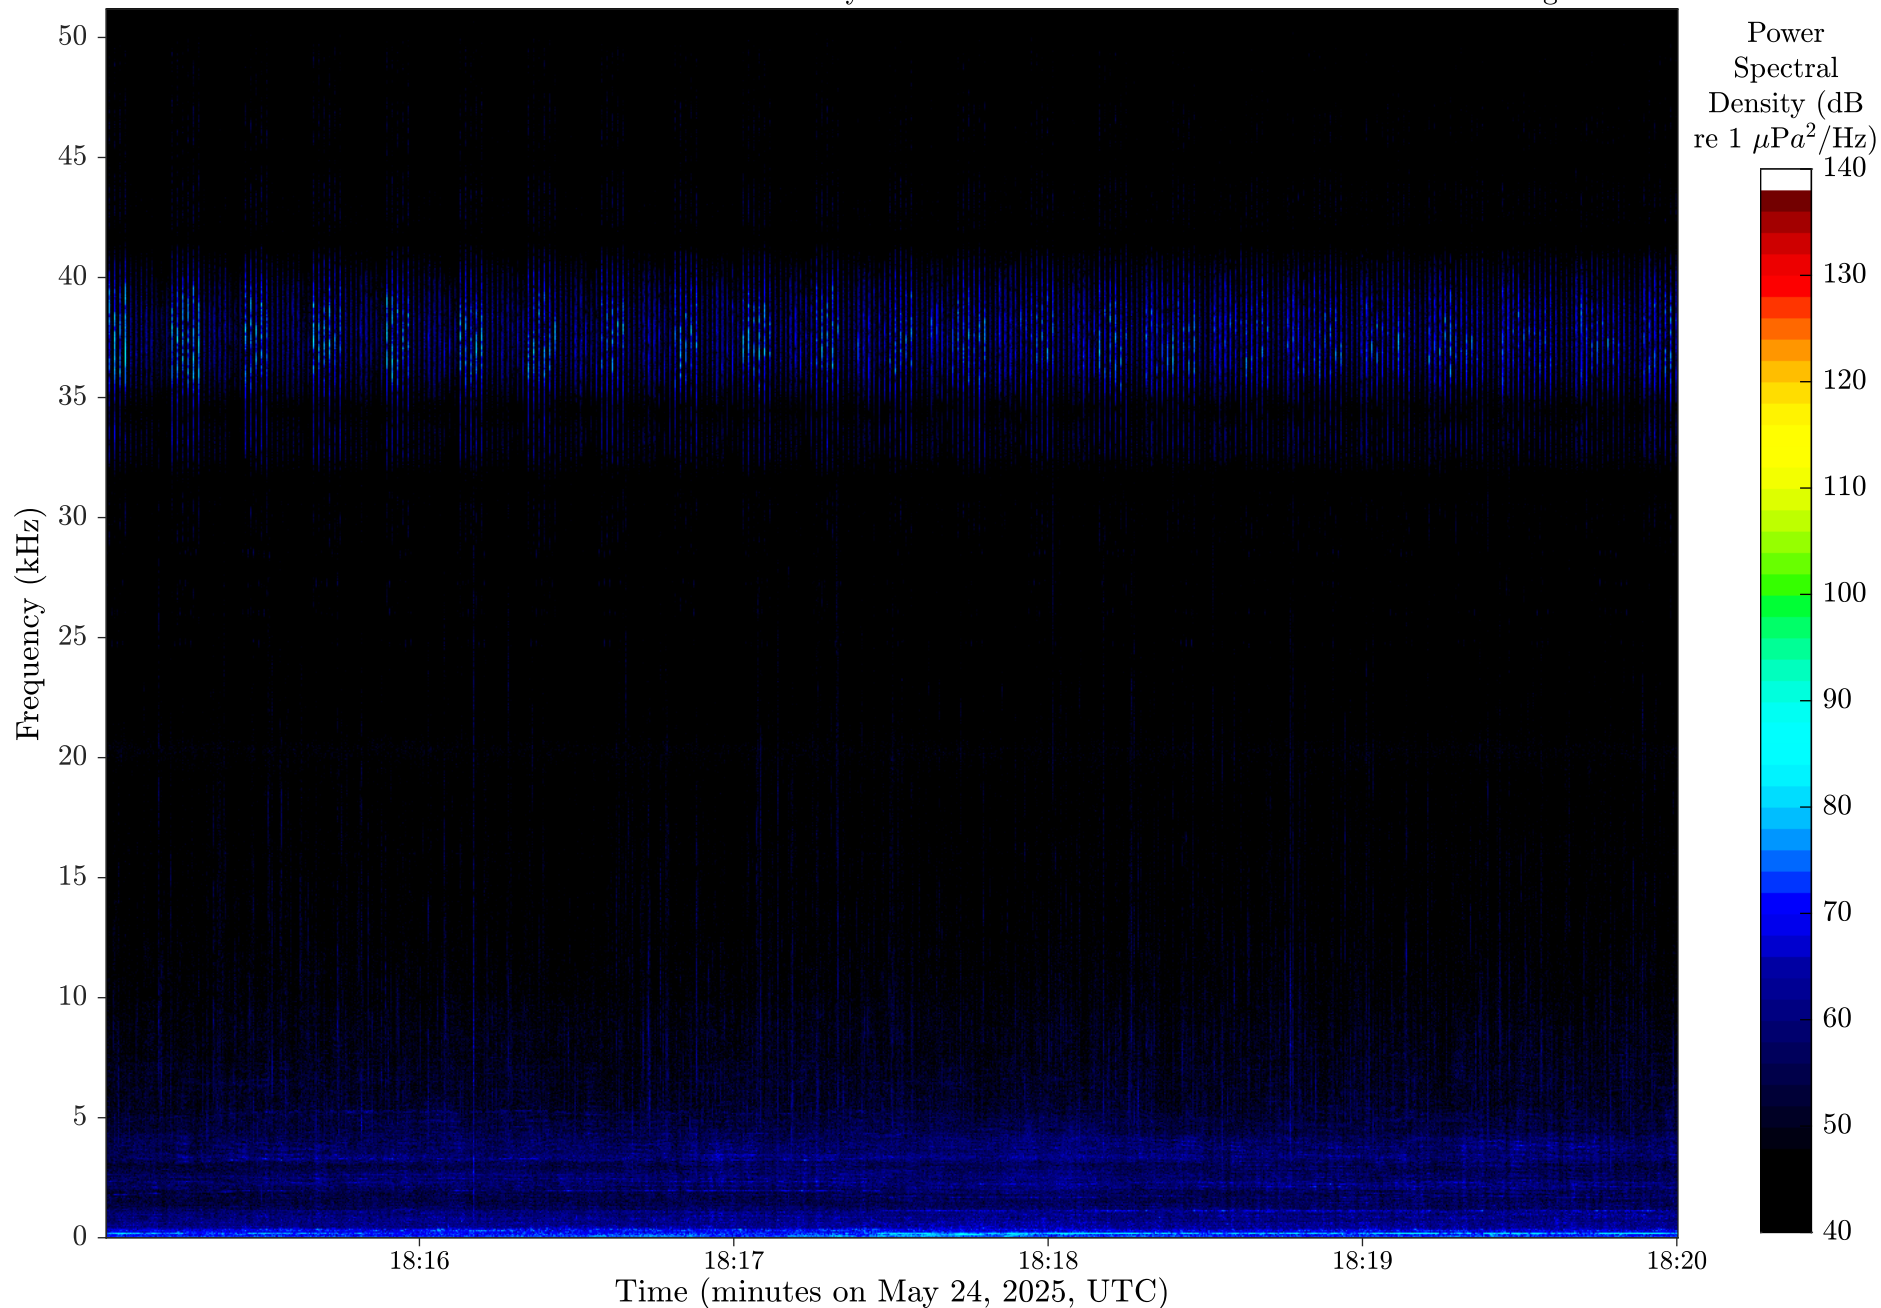

Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:45:25 UTC

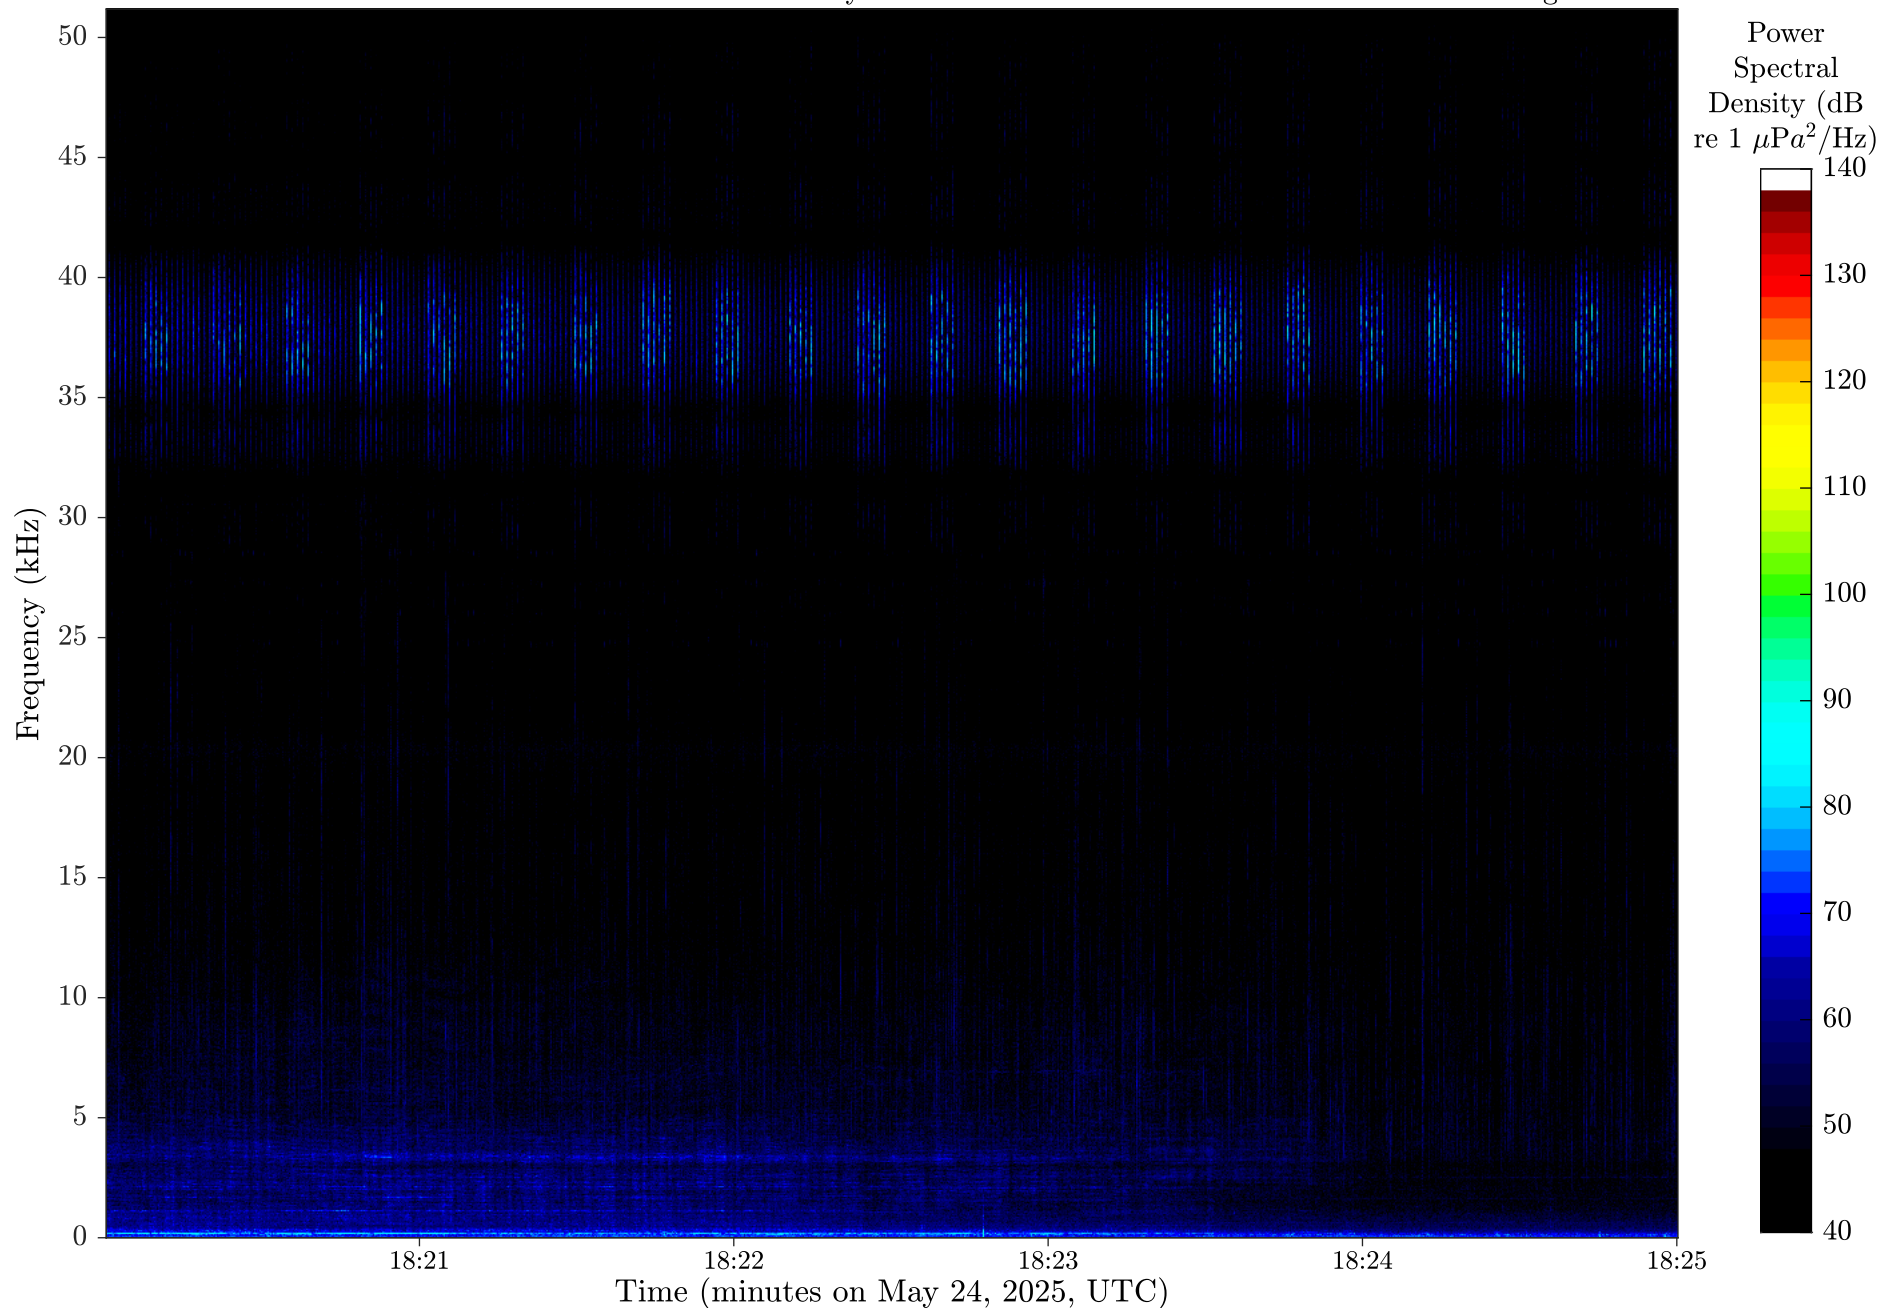

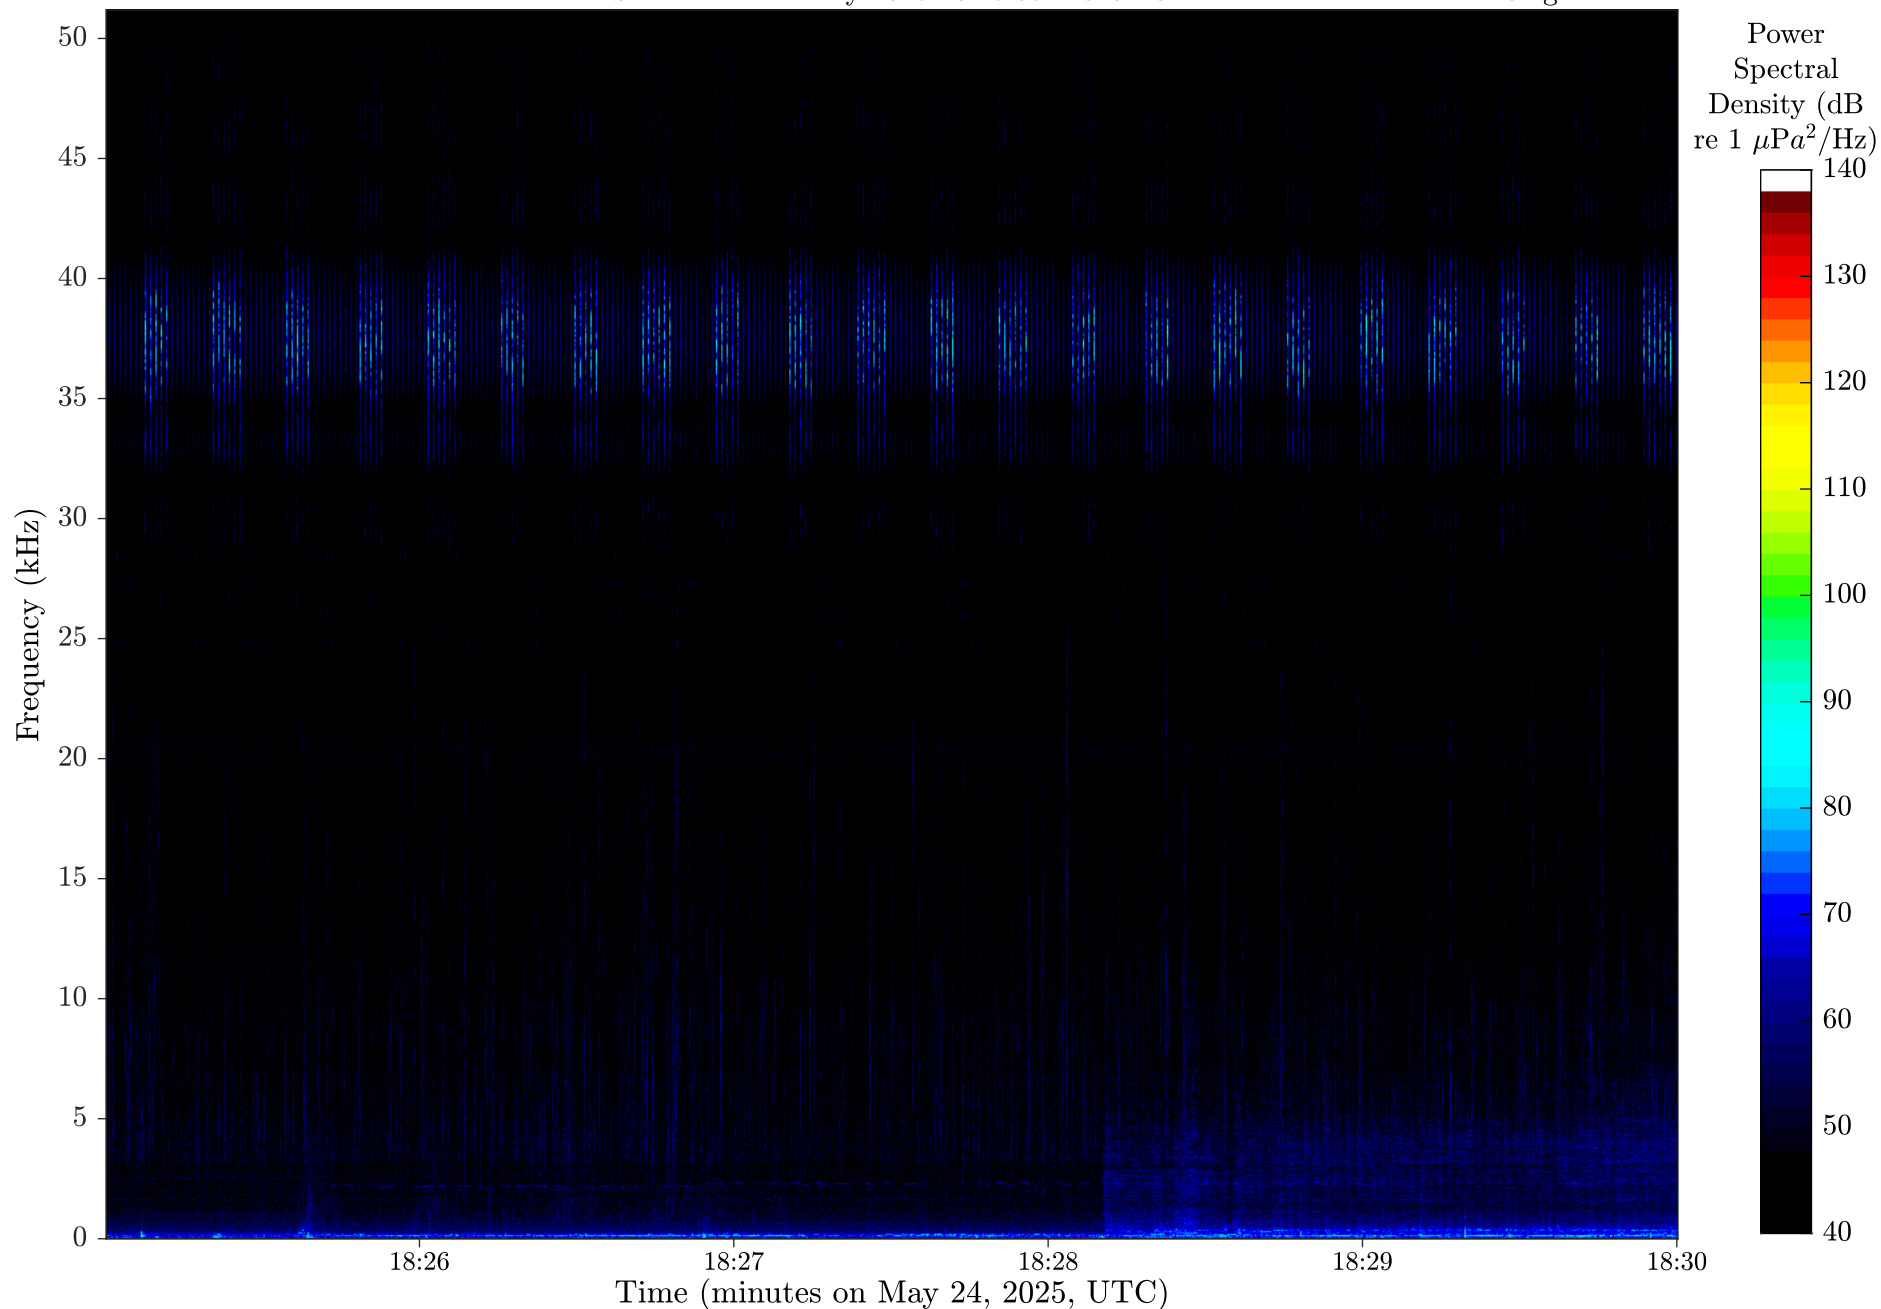


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:45:41 UTC

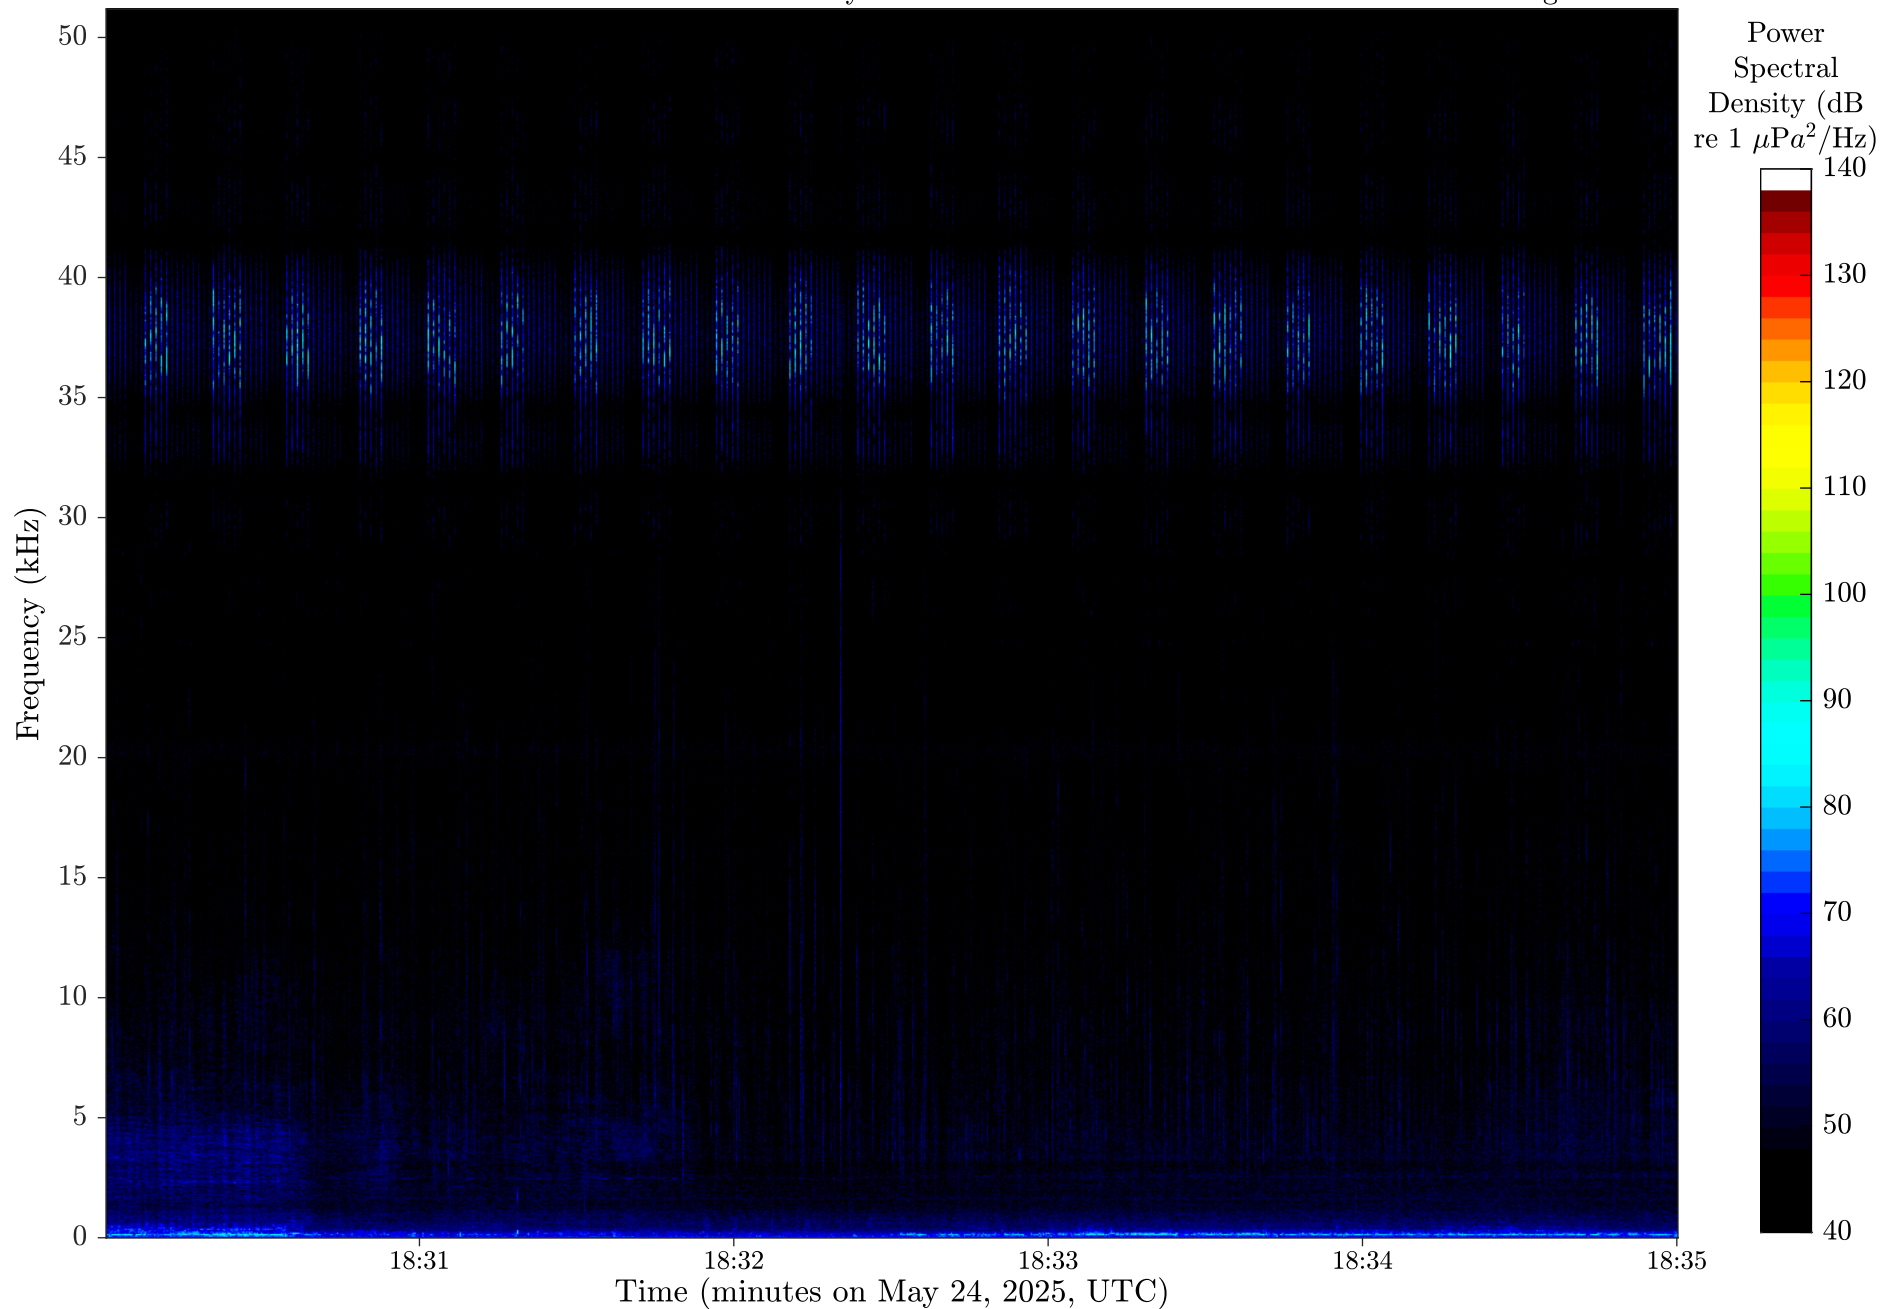


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:45:48 UTC

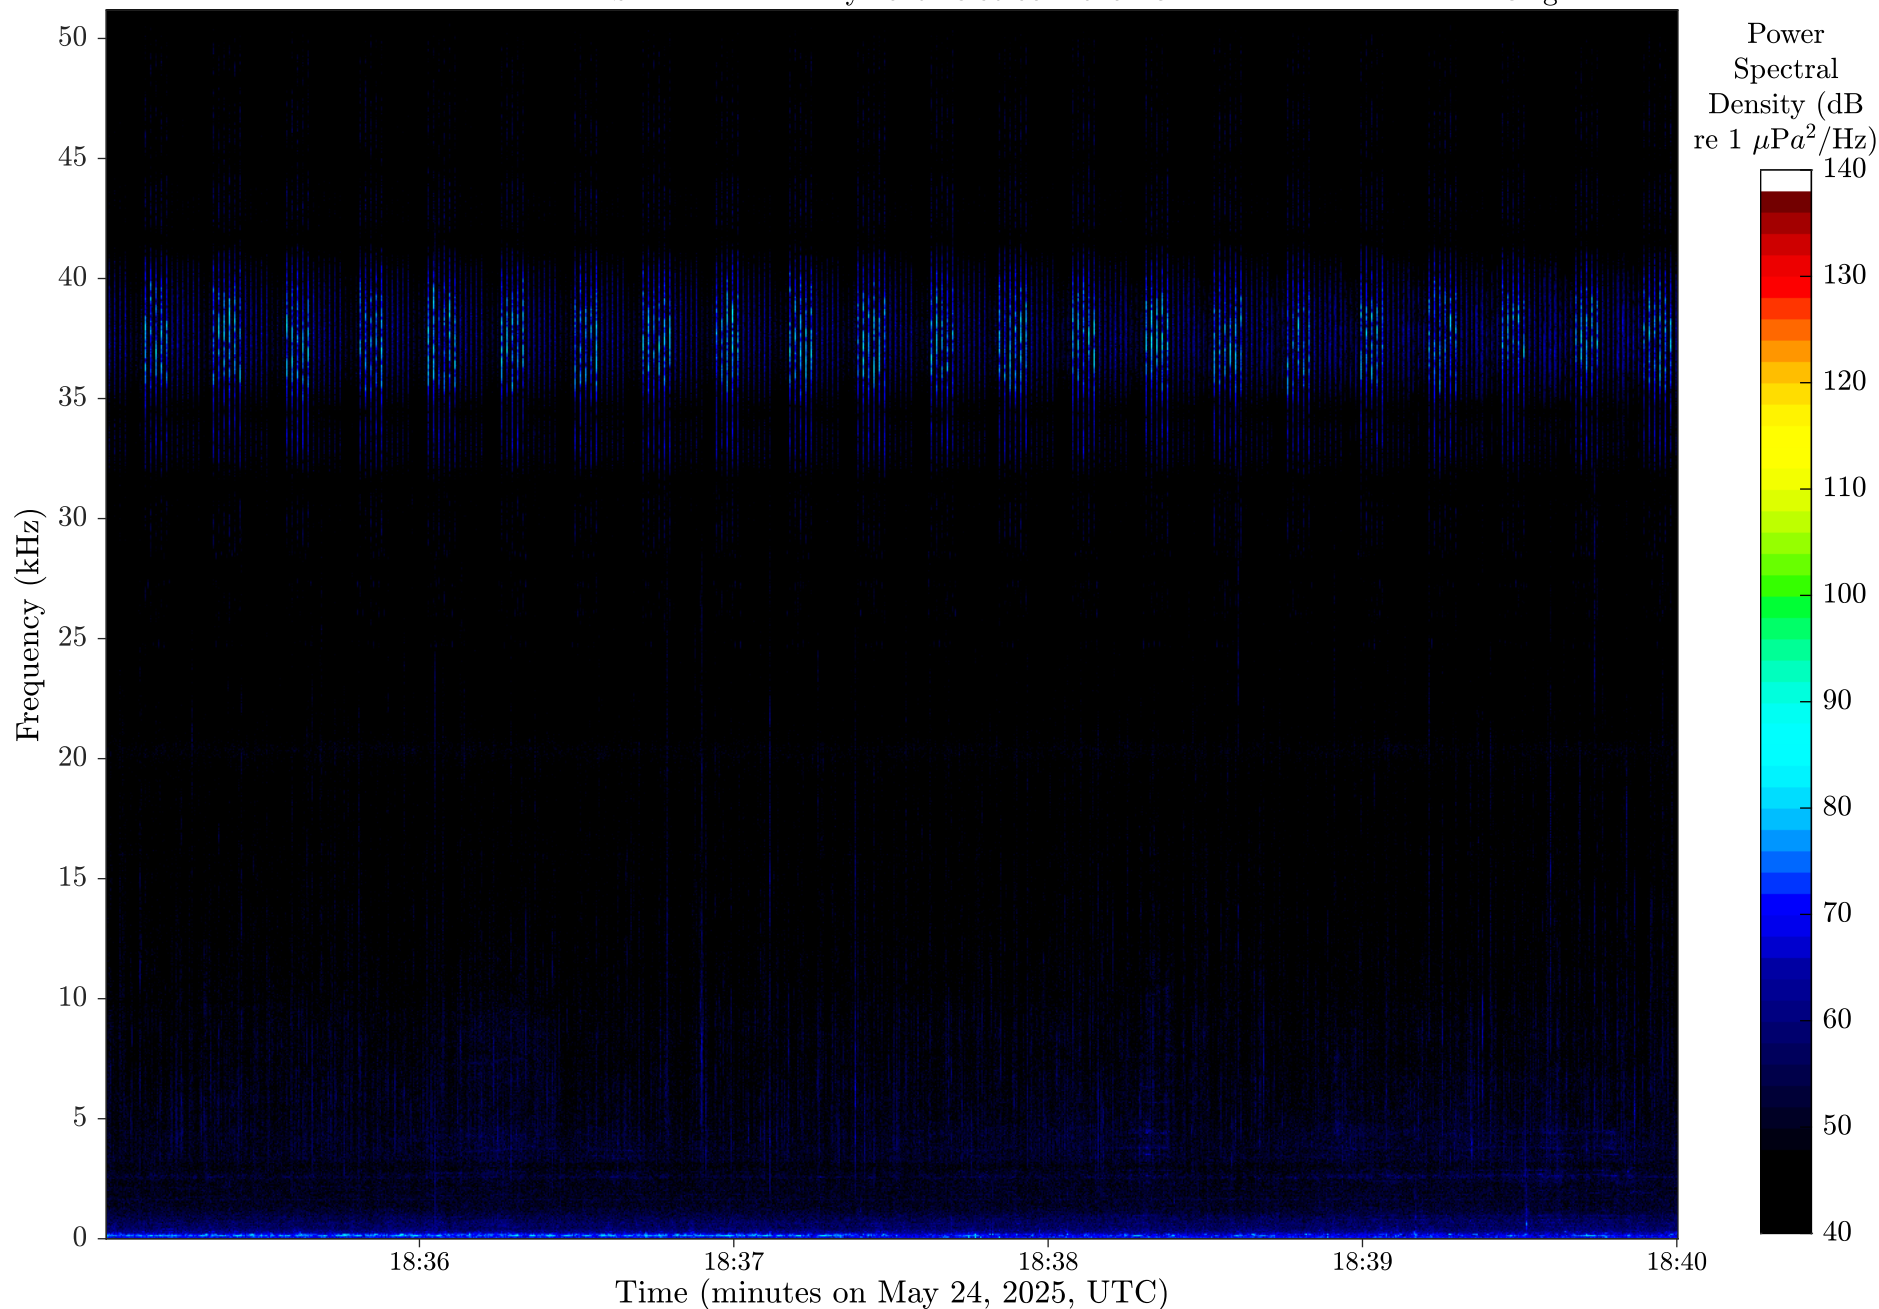


Comments: 31.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:45:57 UTC

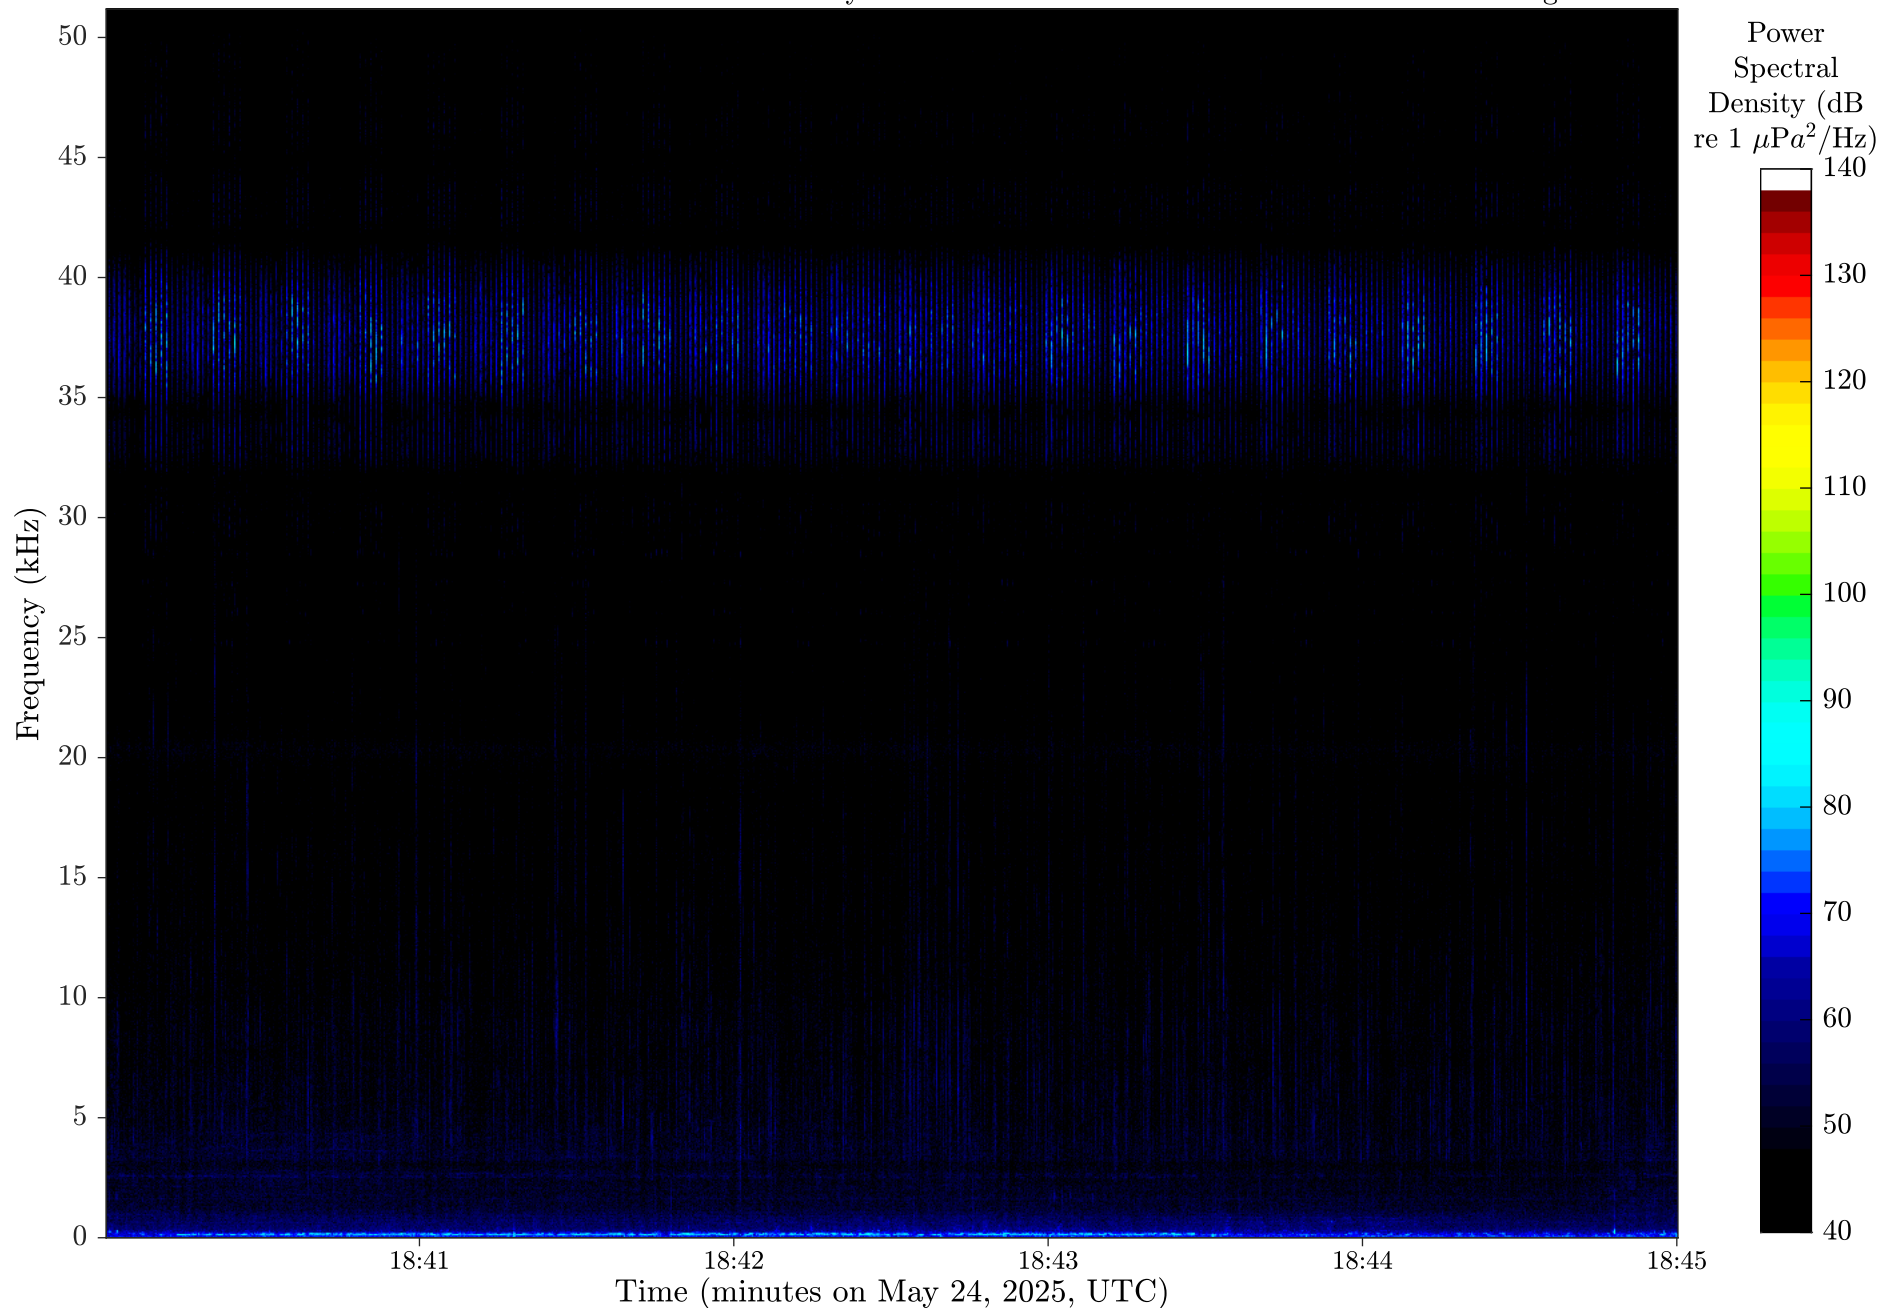


Comments: 30.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:05 UTC

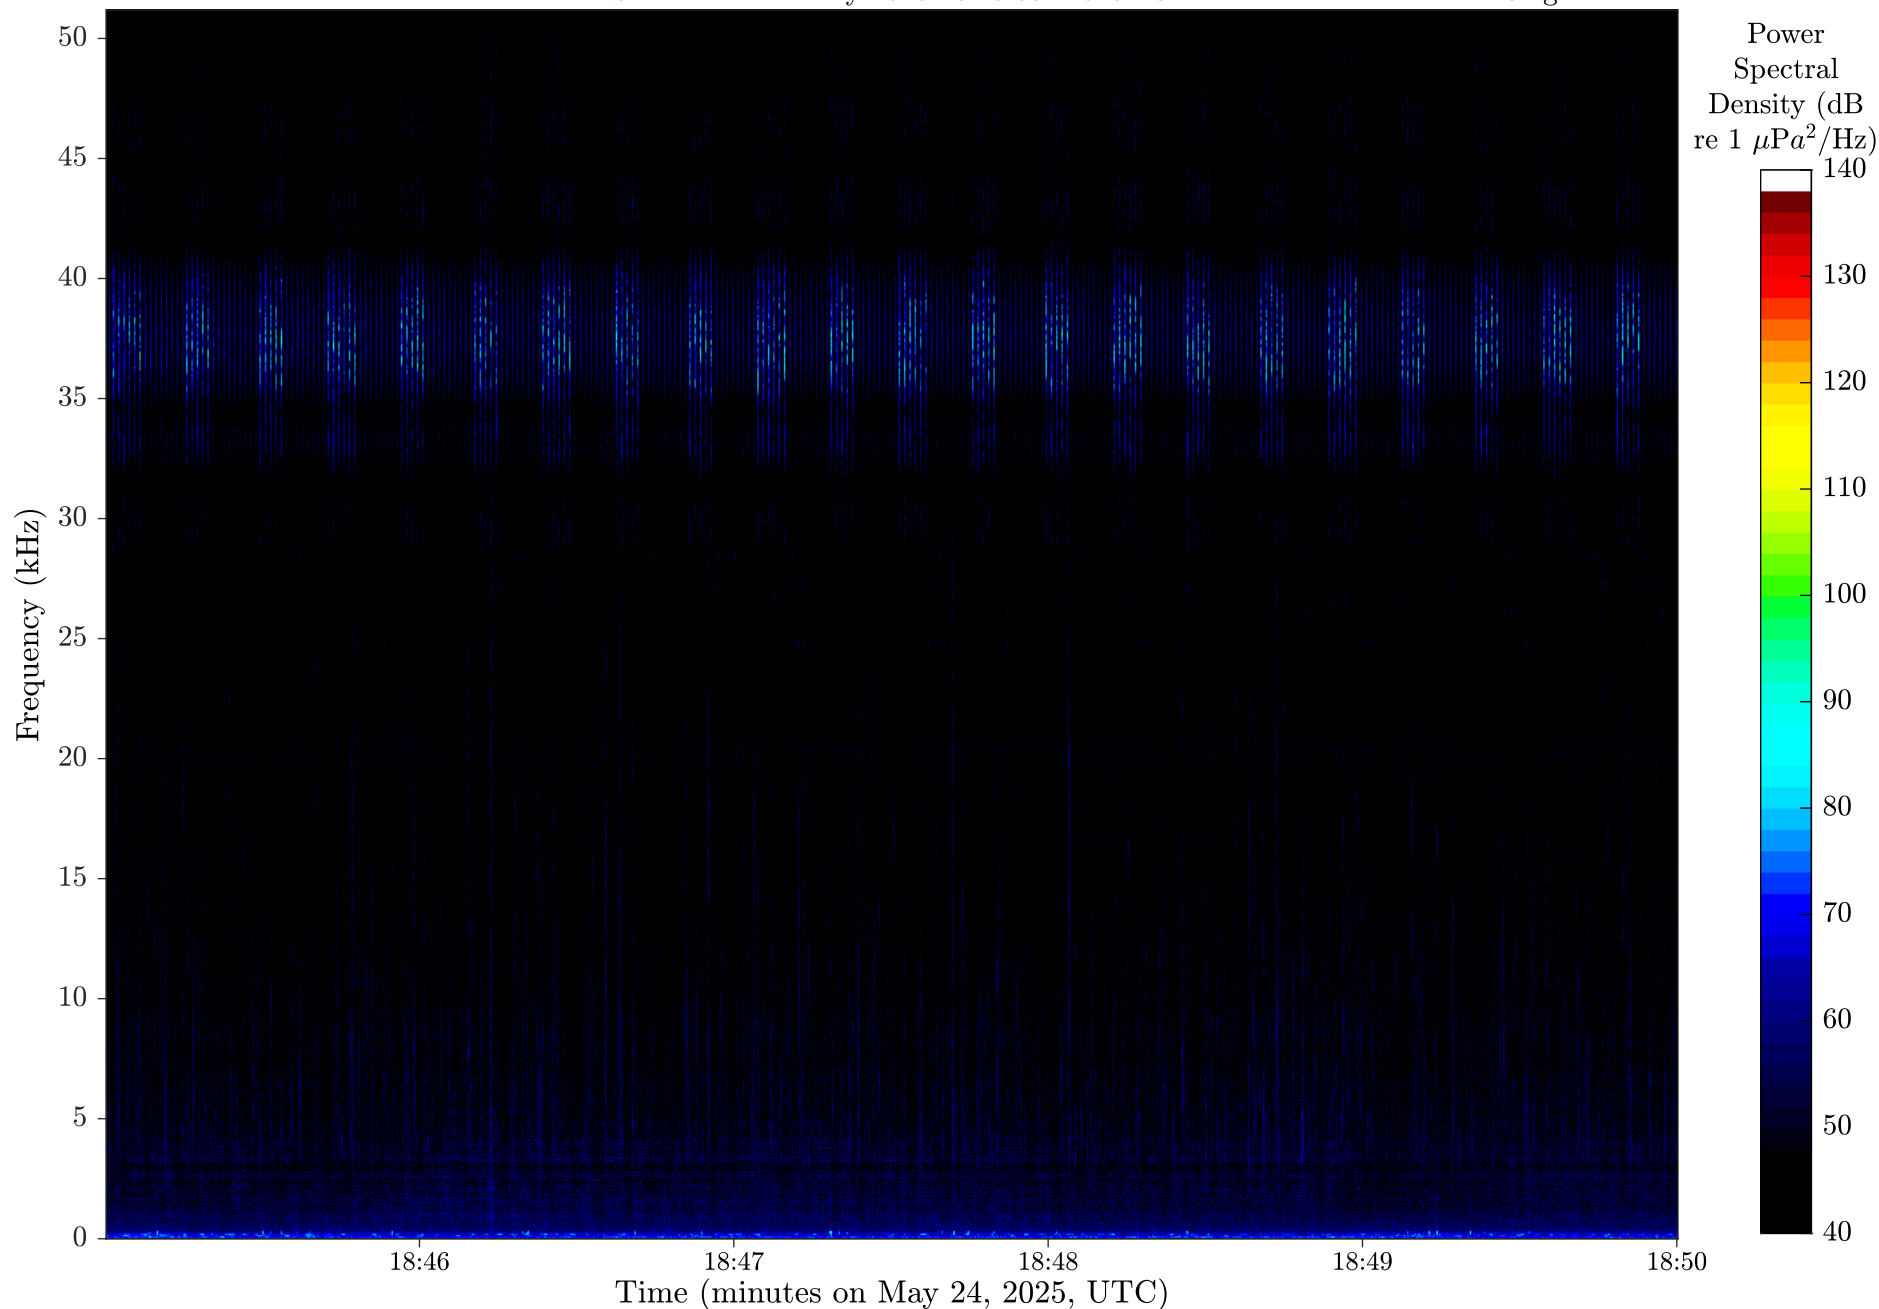


Comments: 31.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:13 UTC

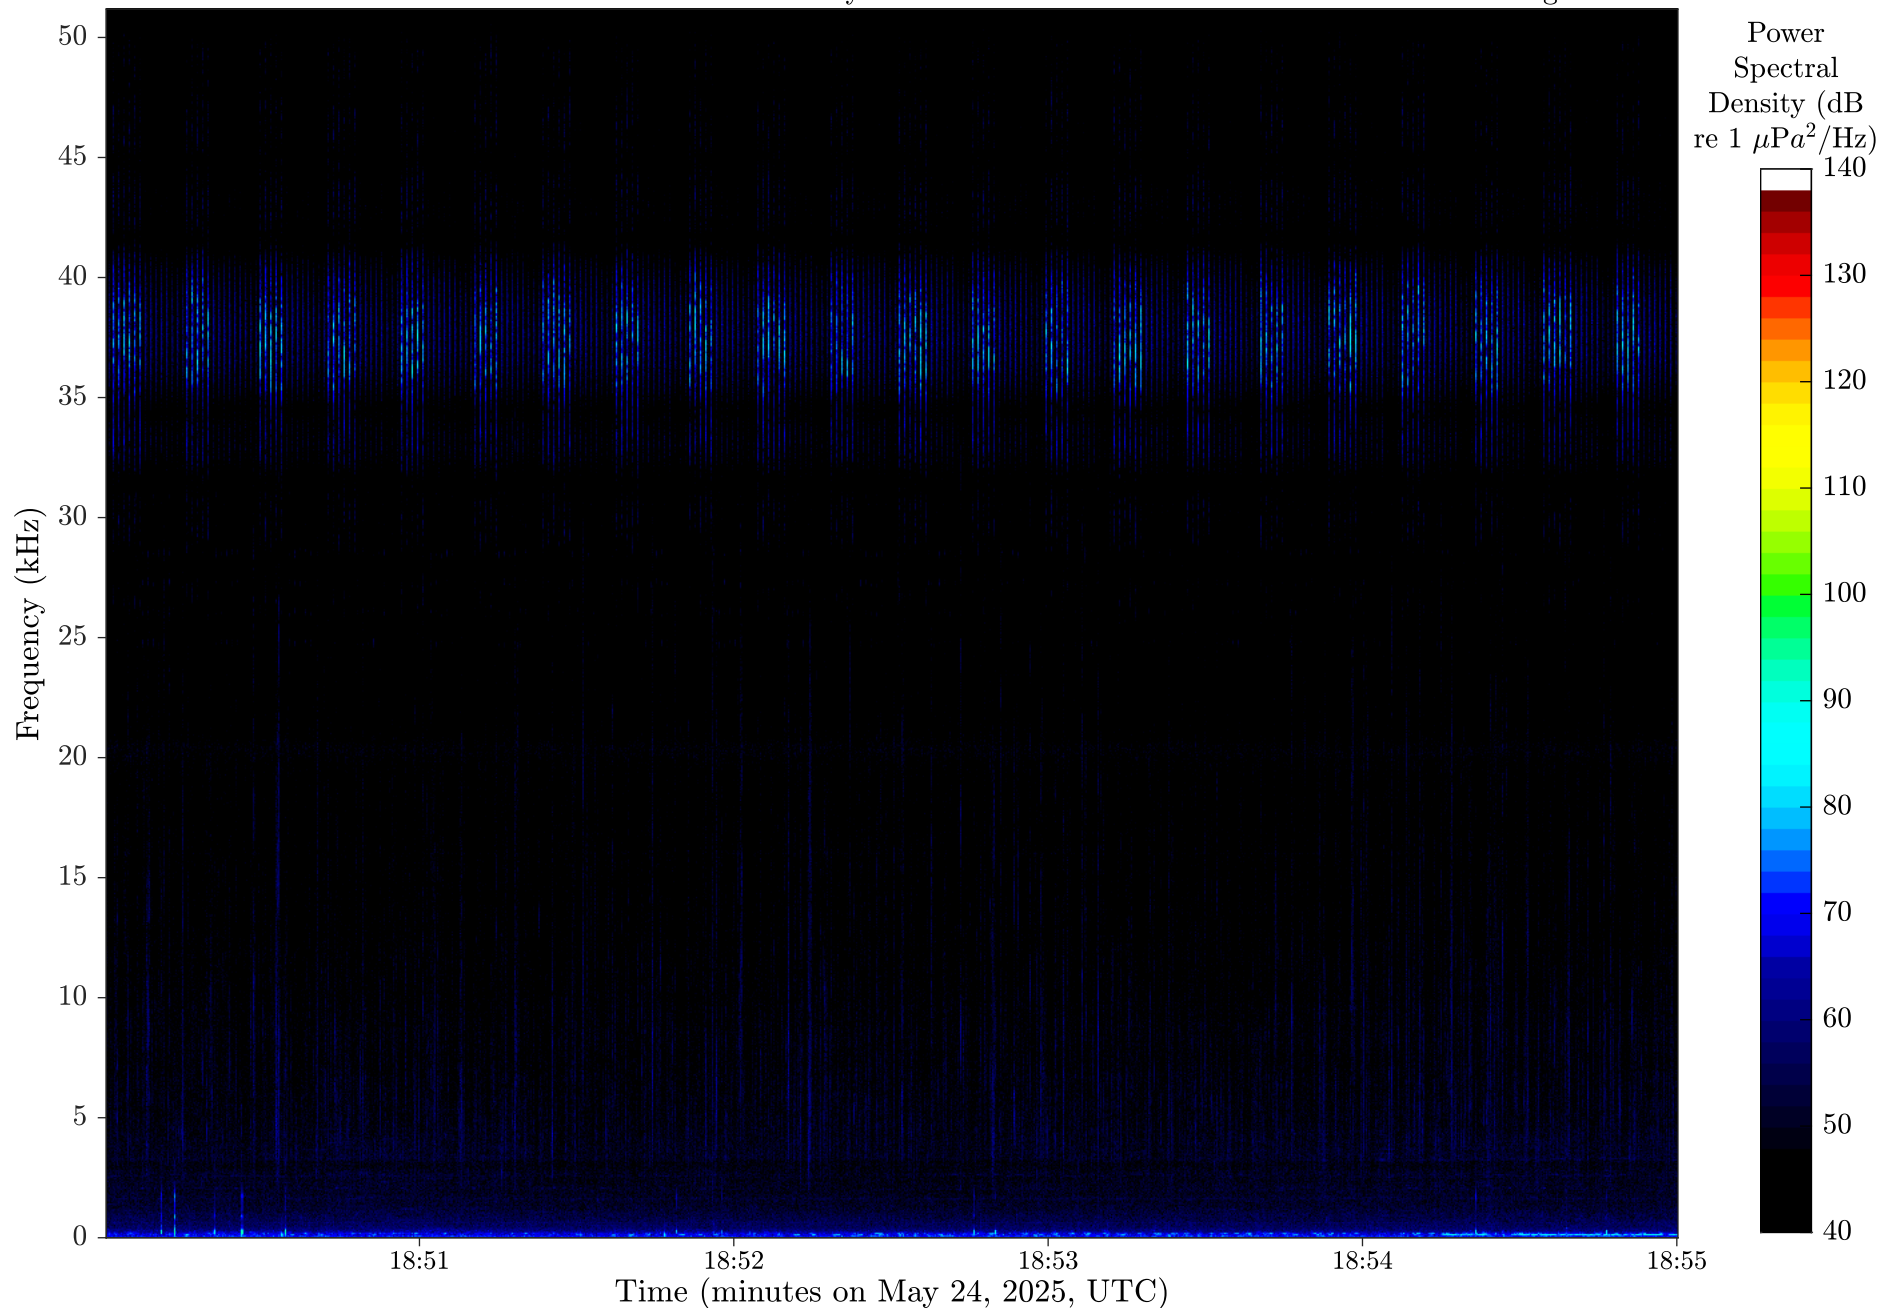


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:21 UTC

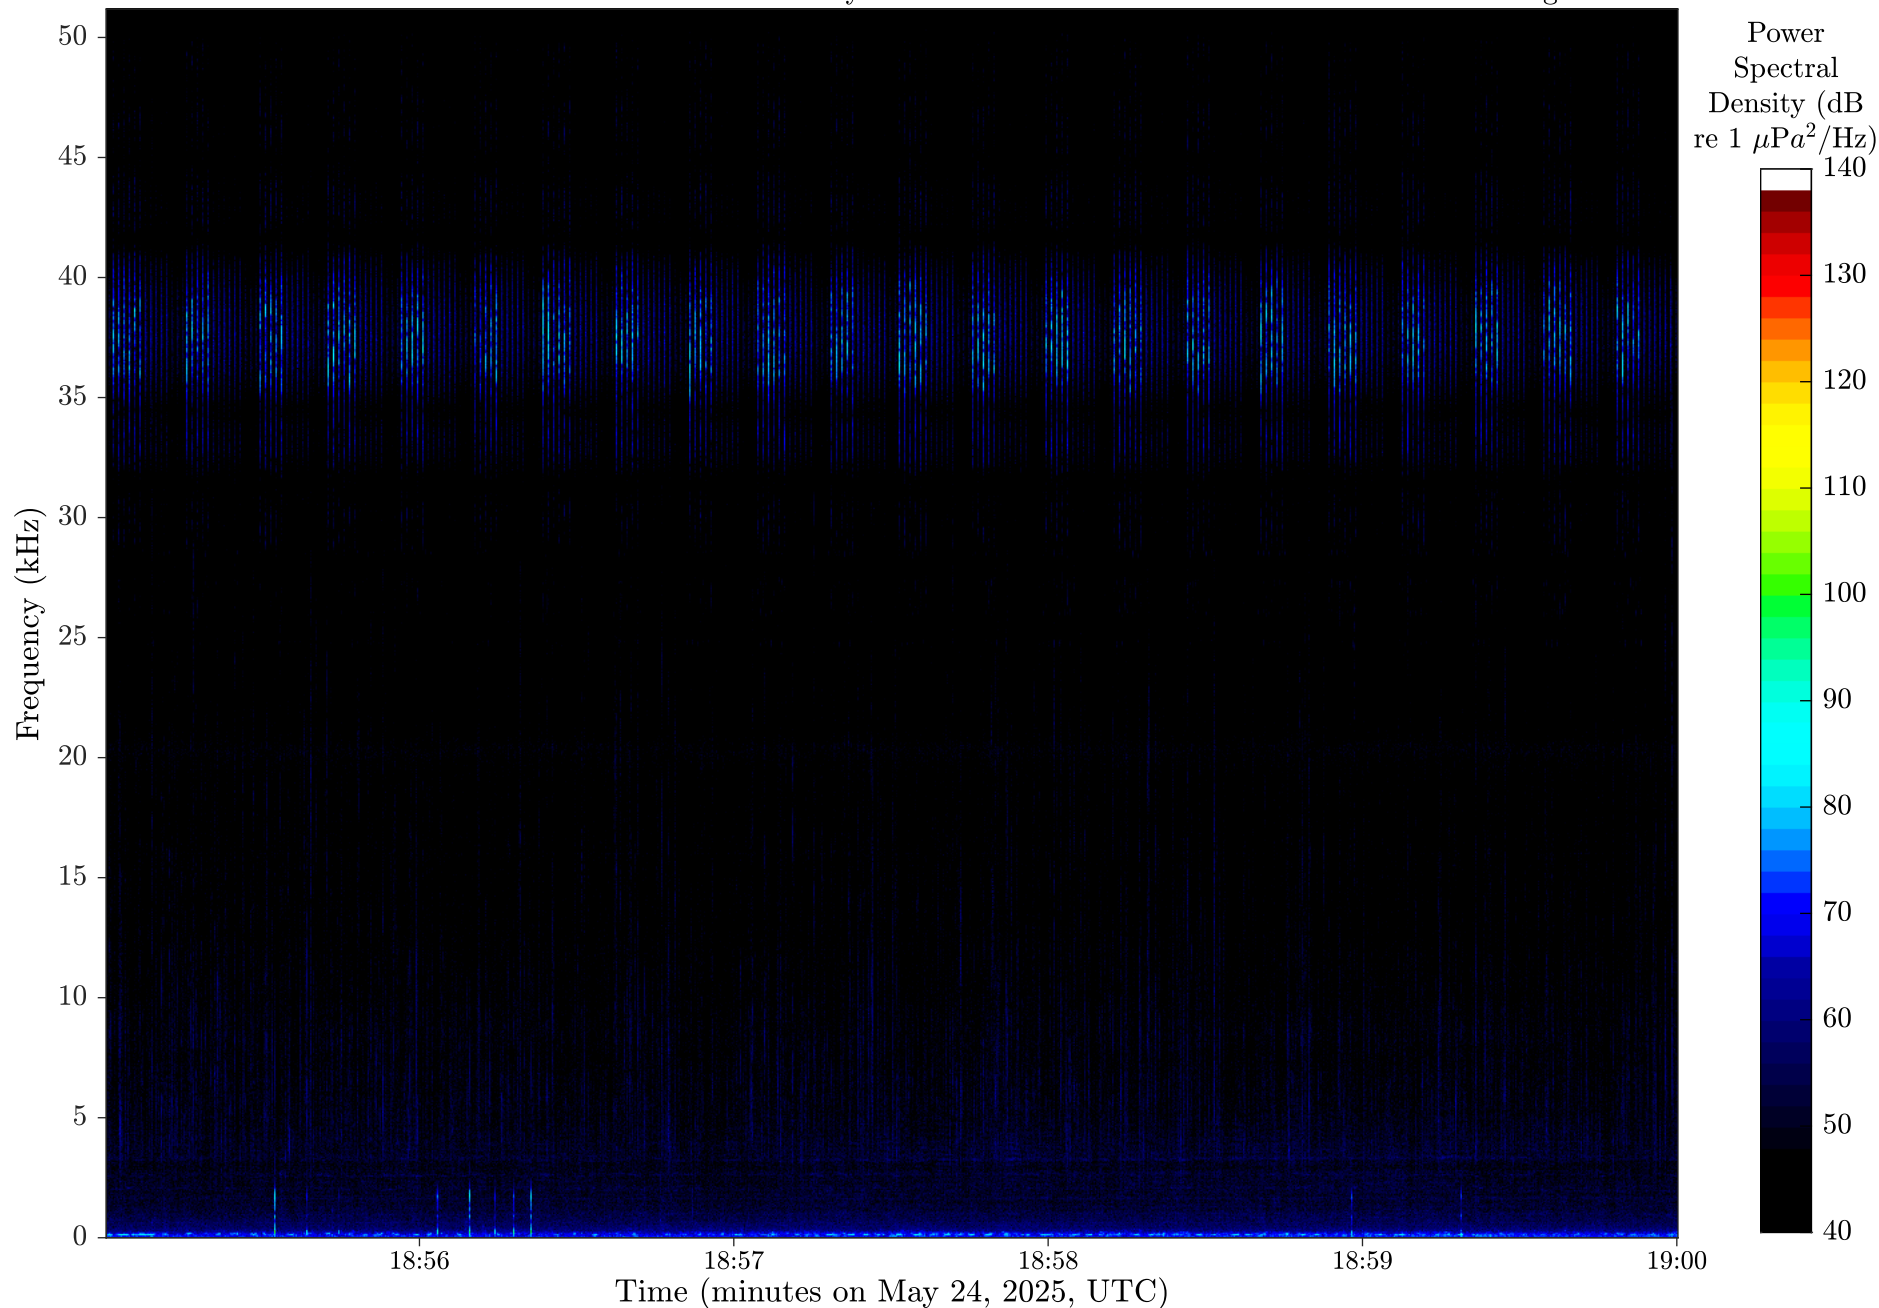


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:29 UTC

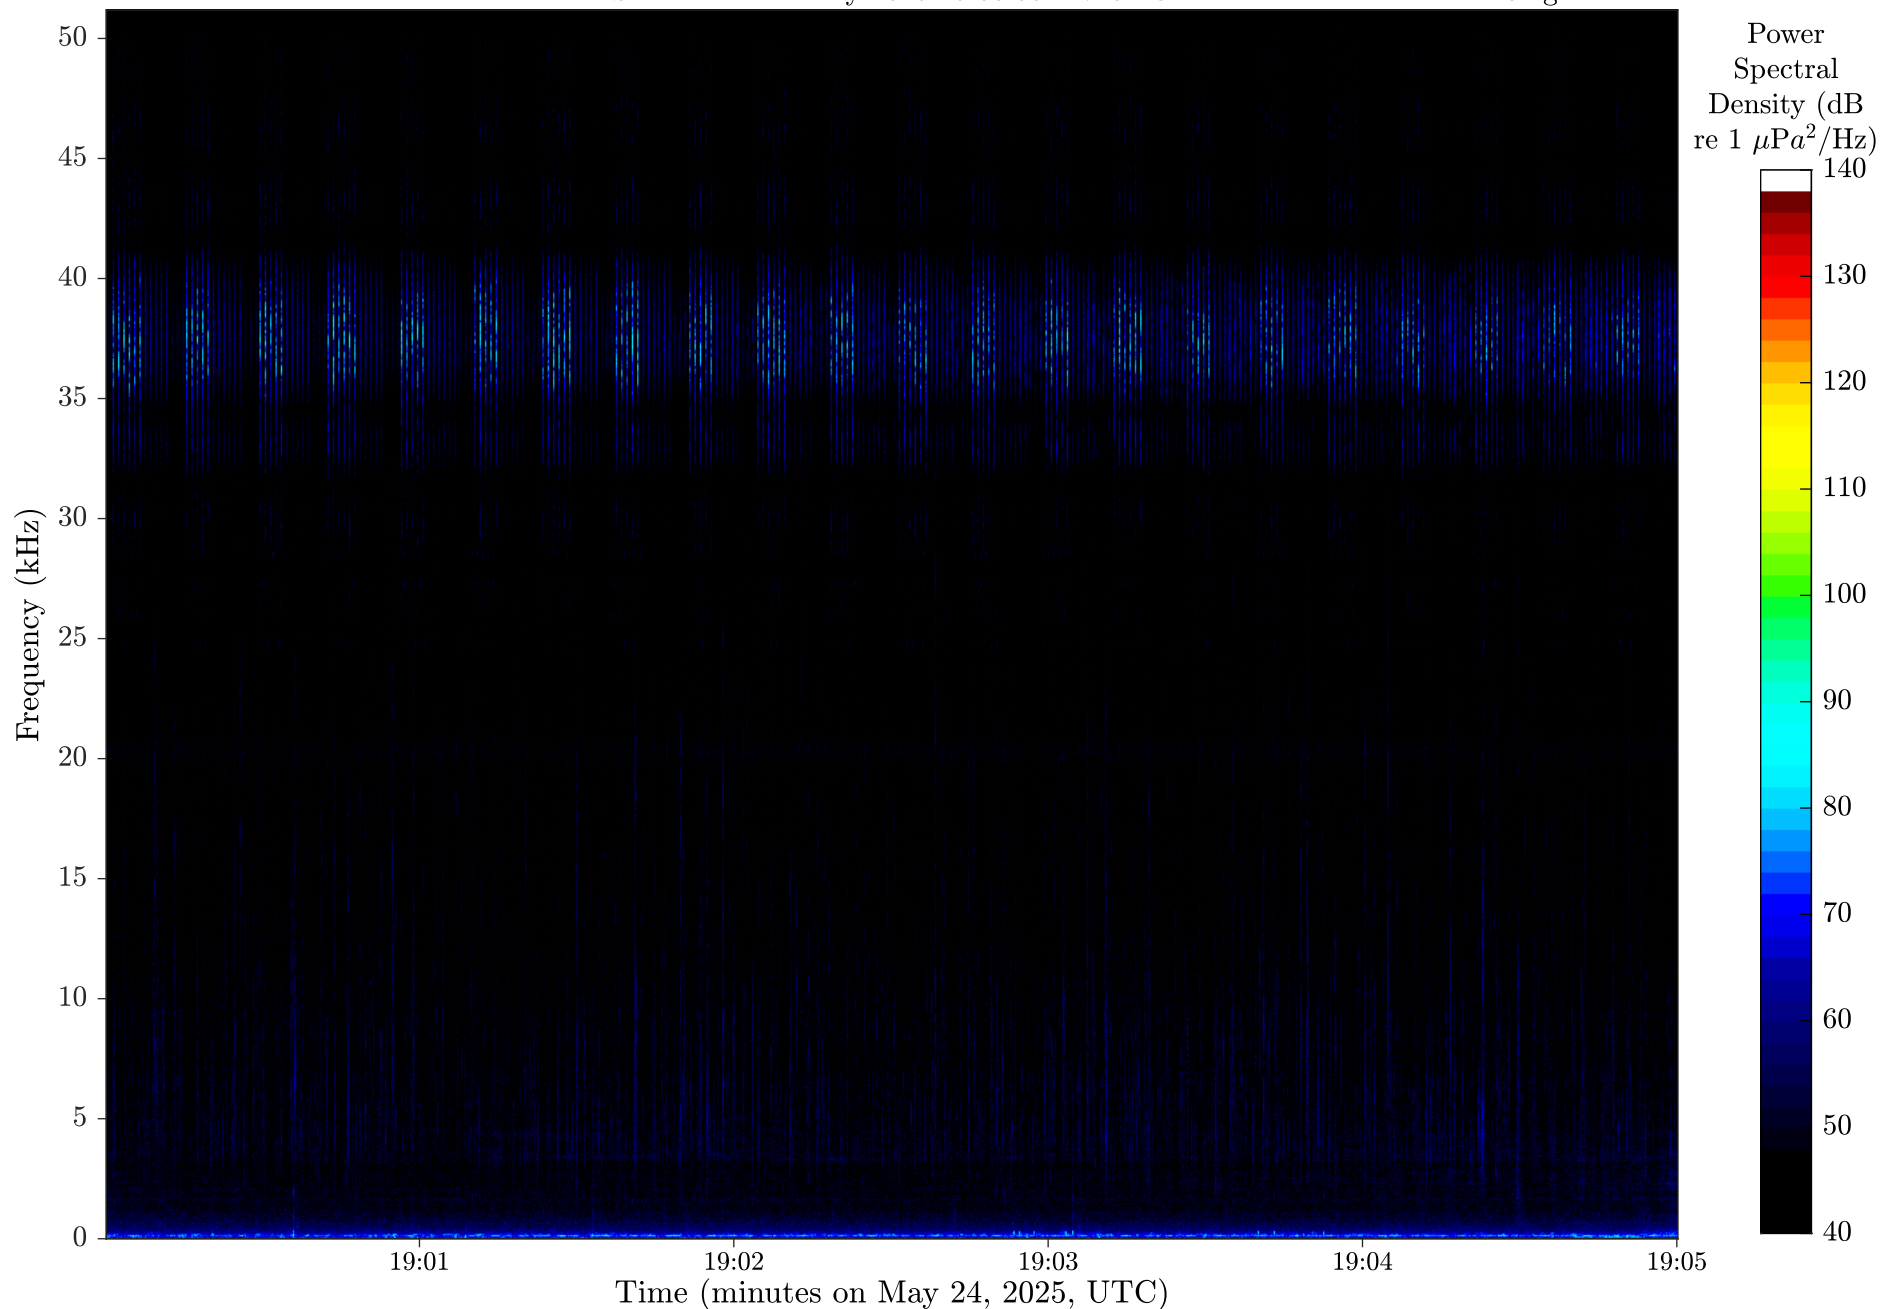


Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:36 UTC

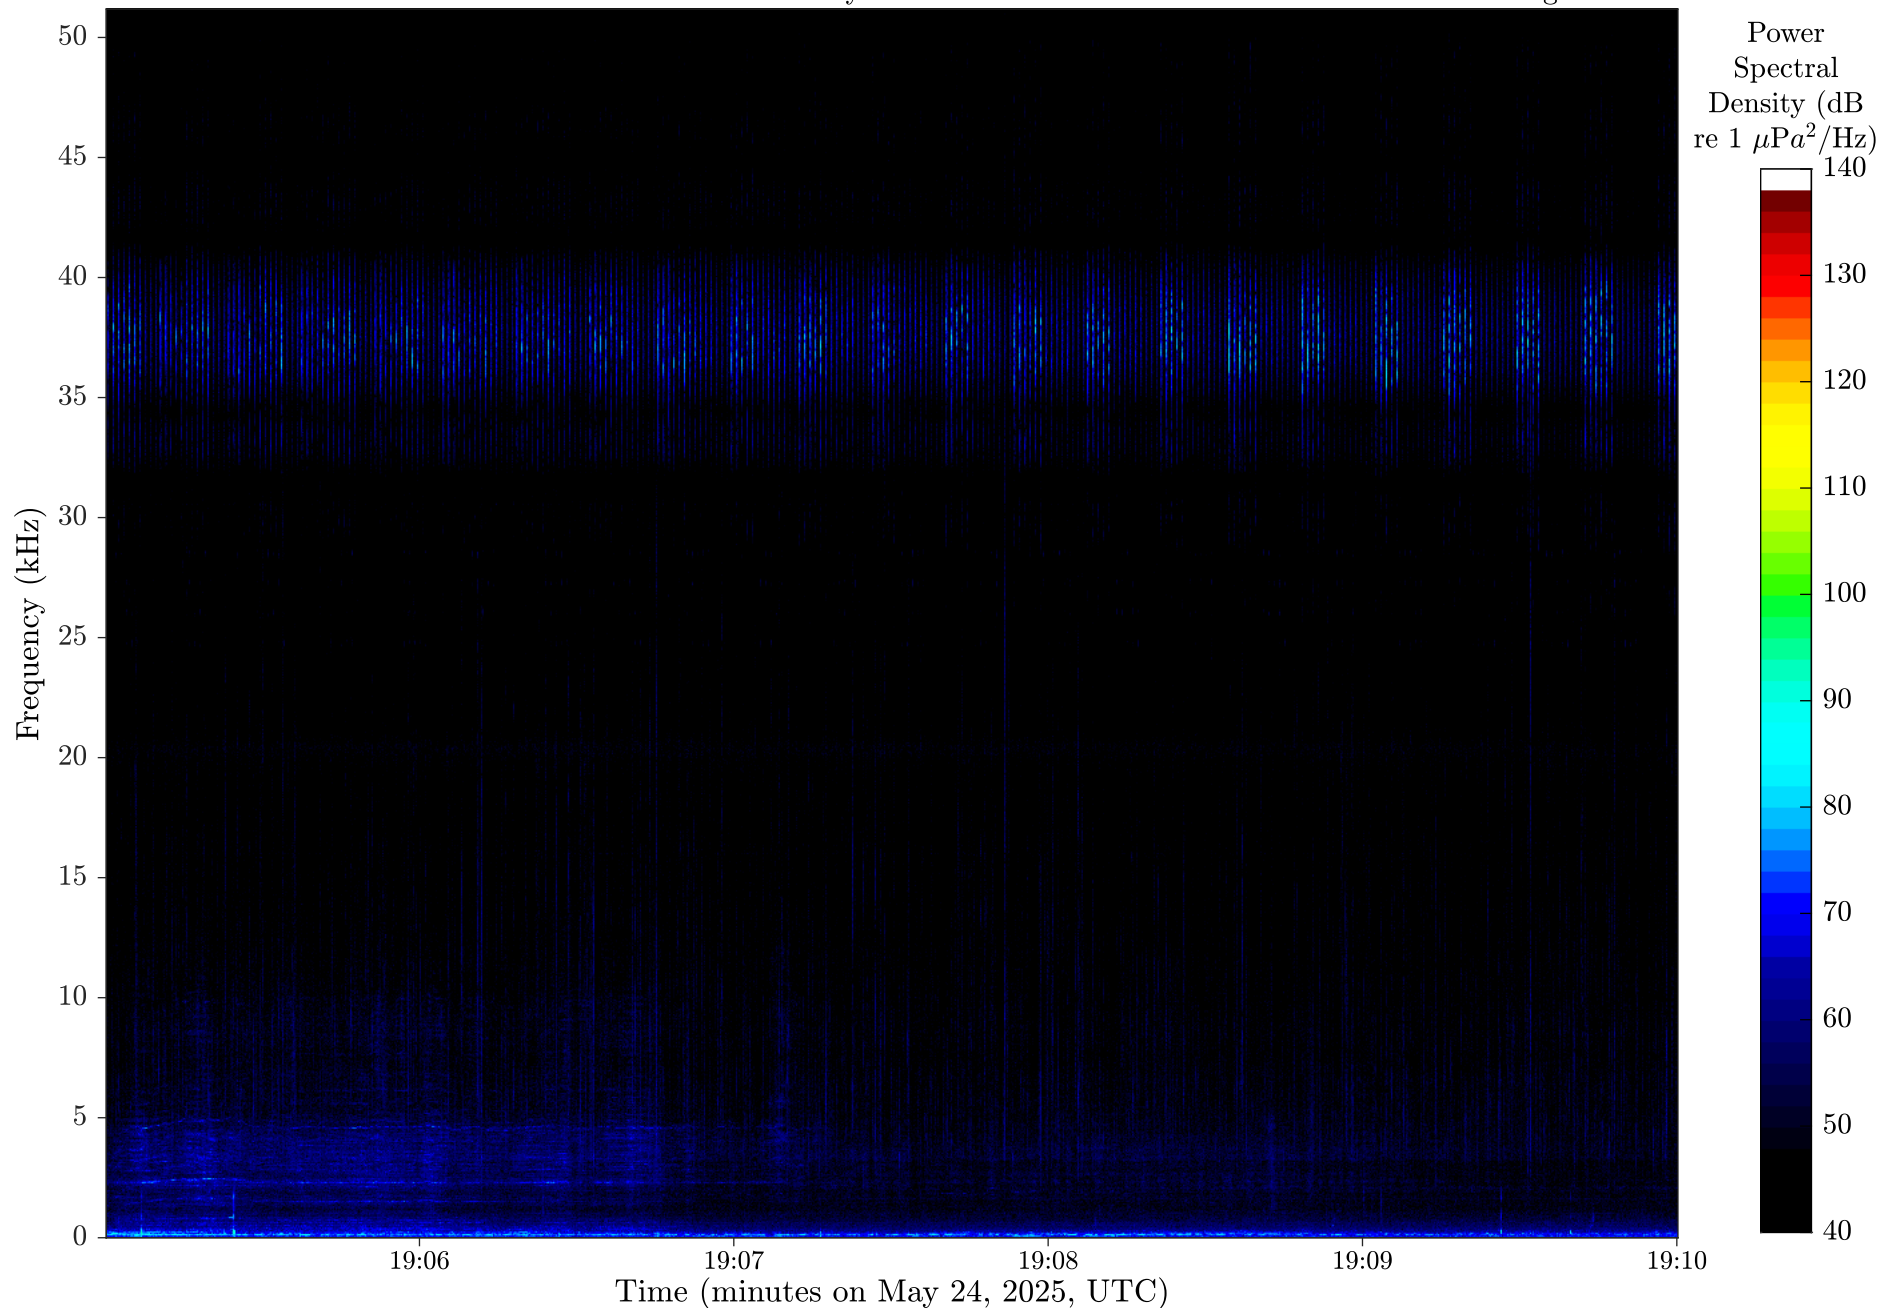


Comments: 32.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:44 UTC

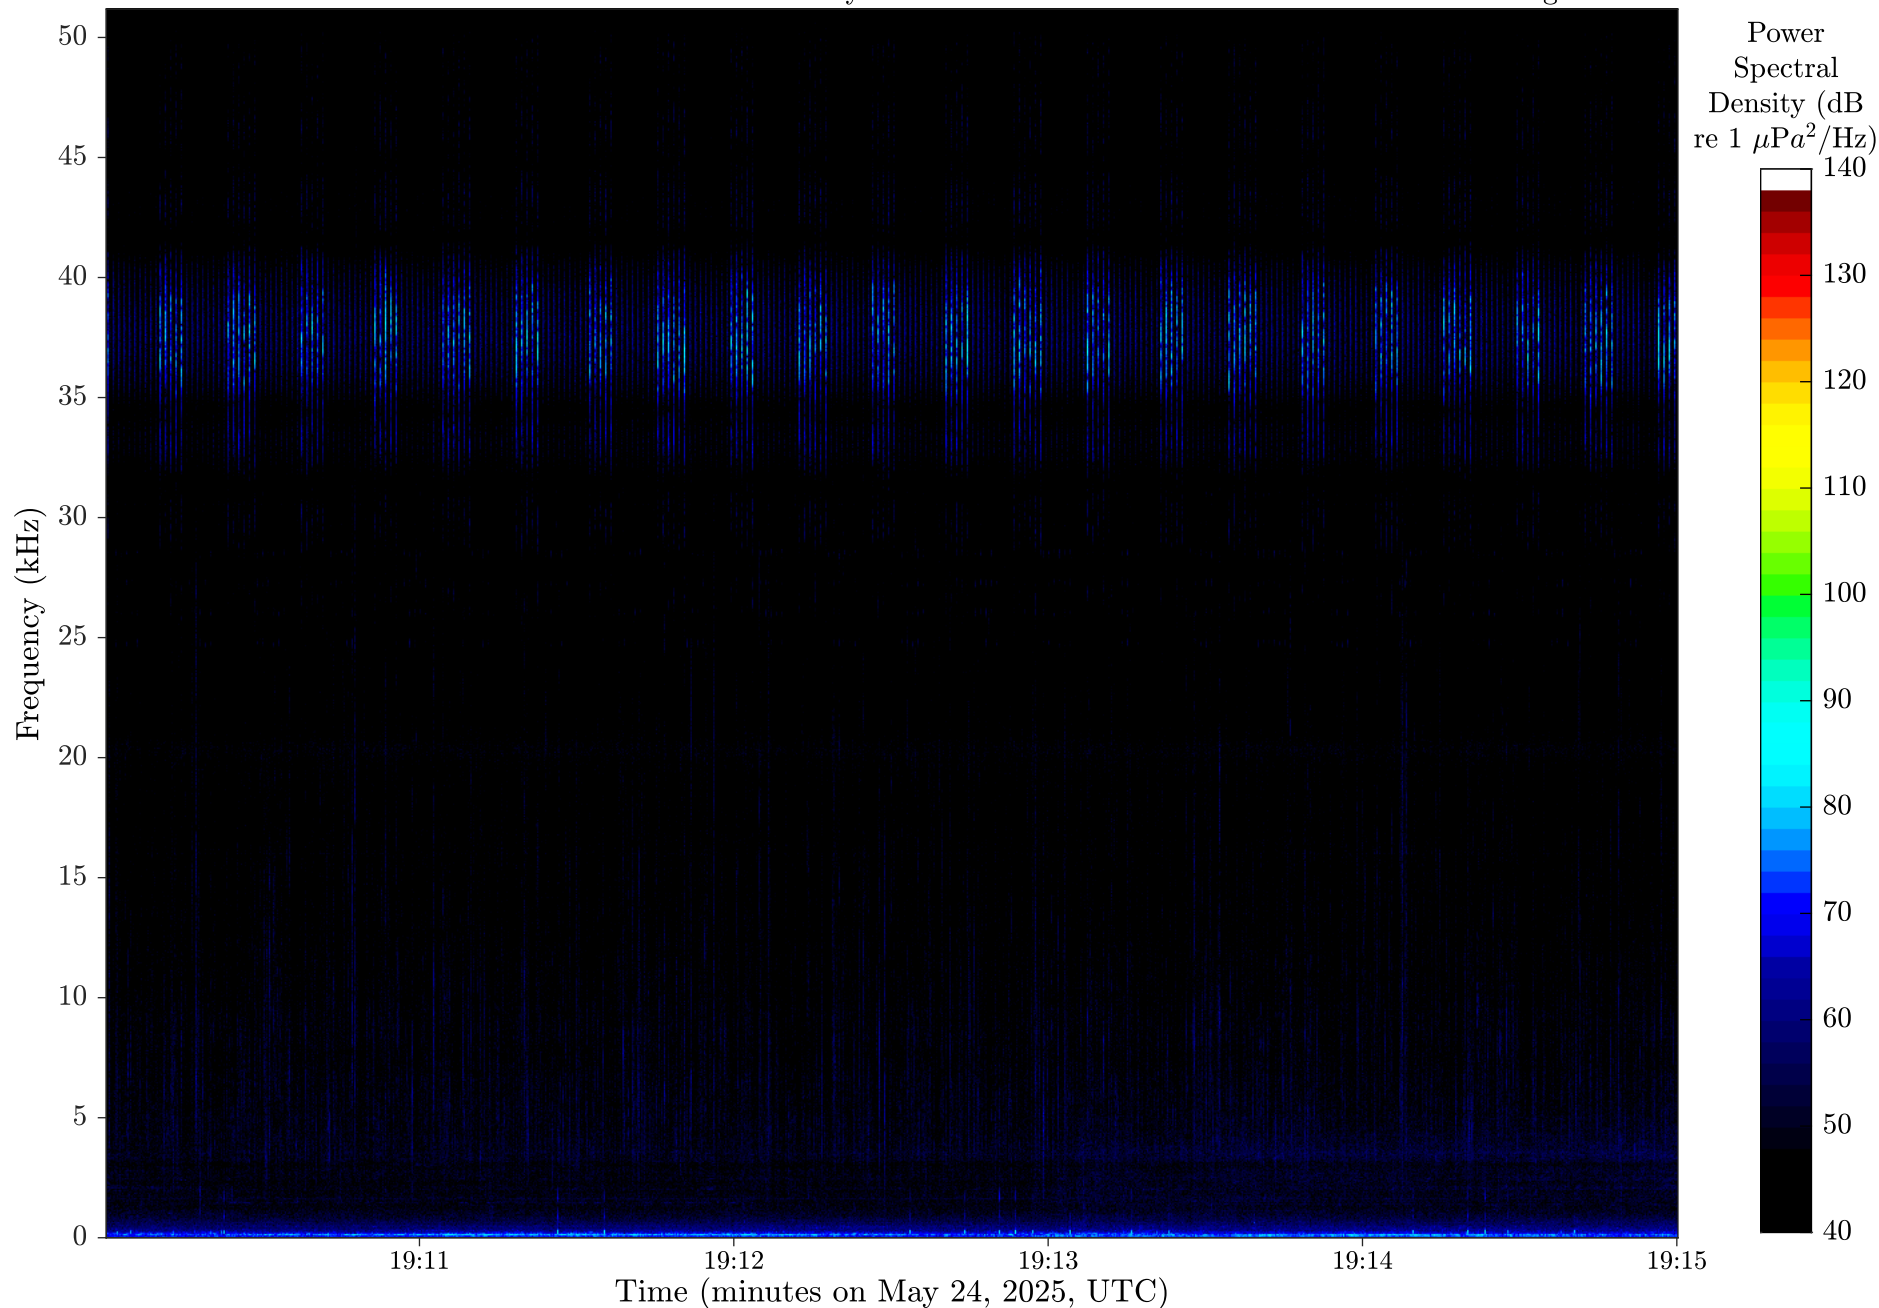


Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:52 UTC

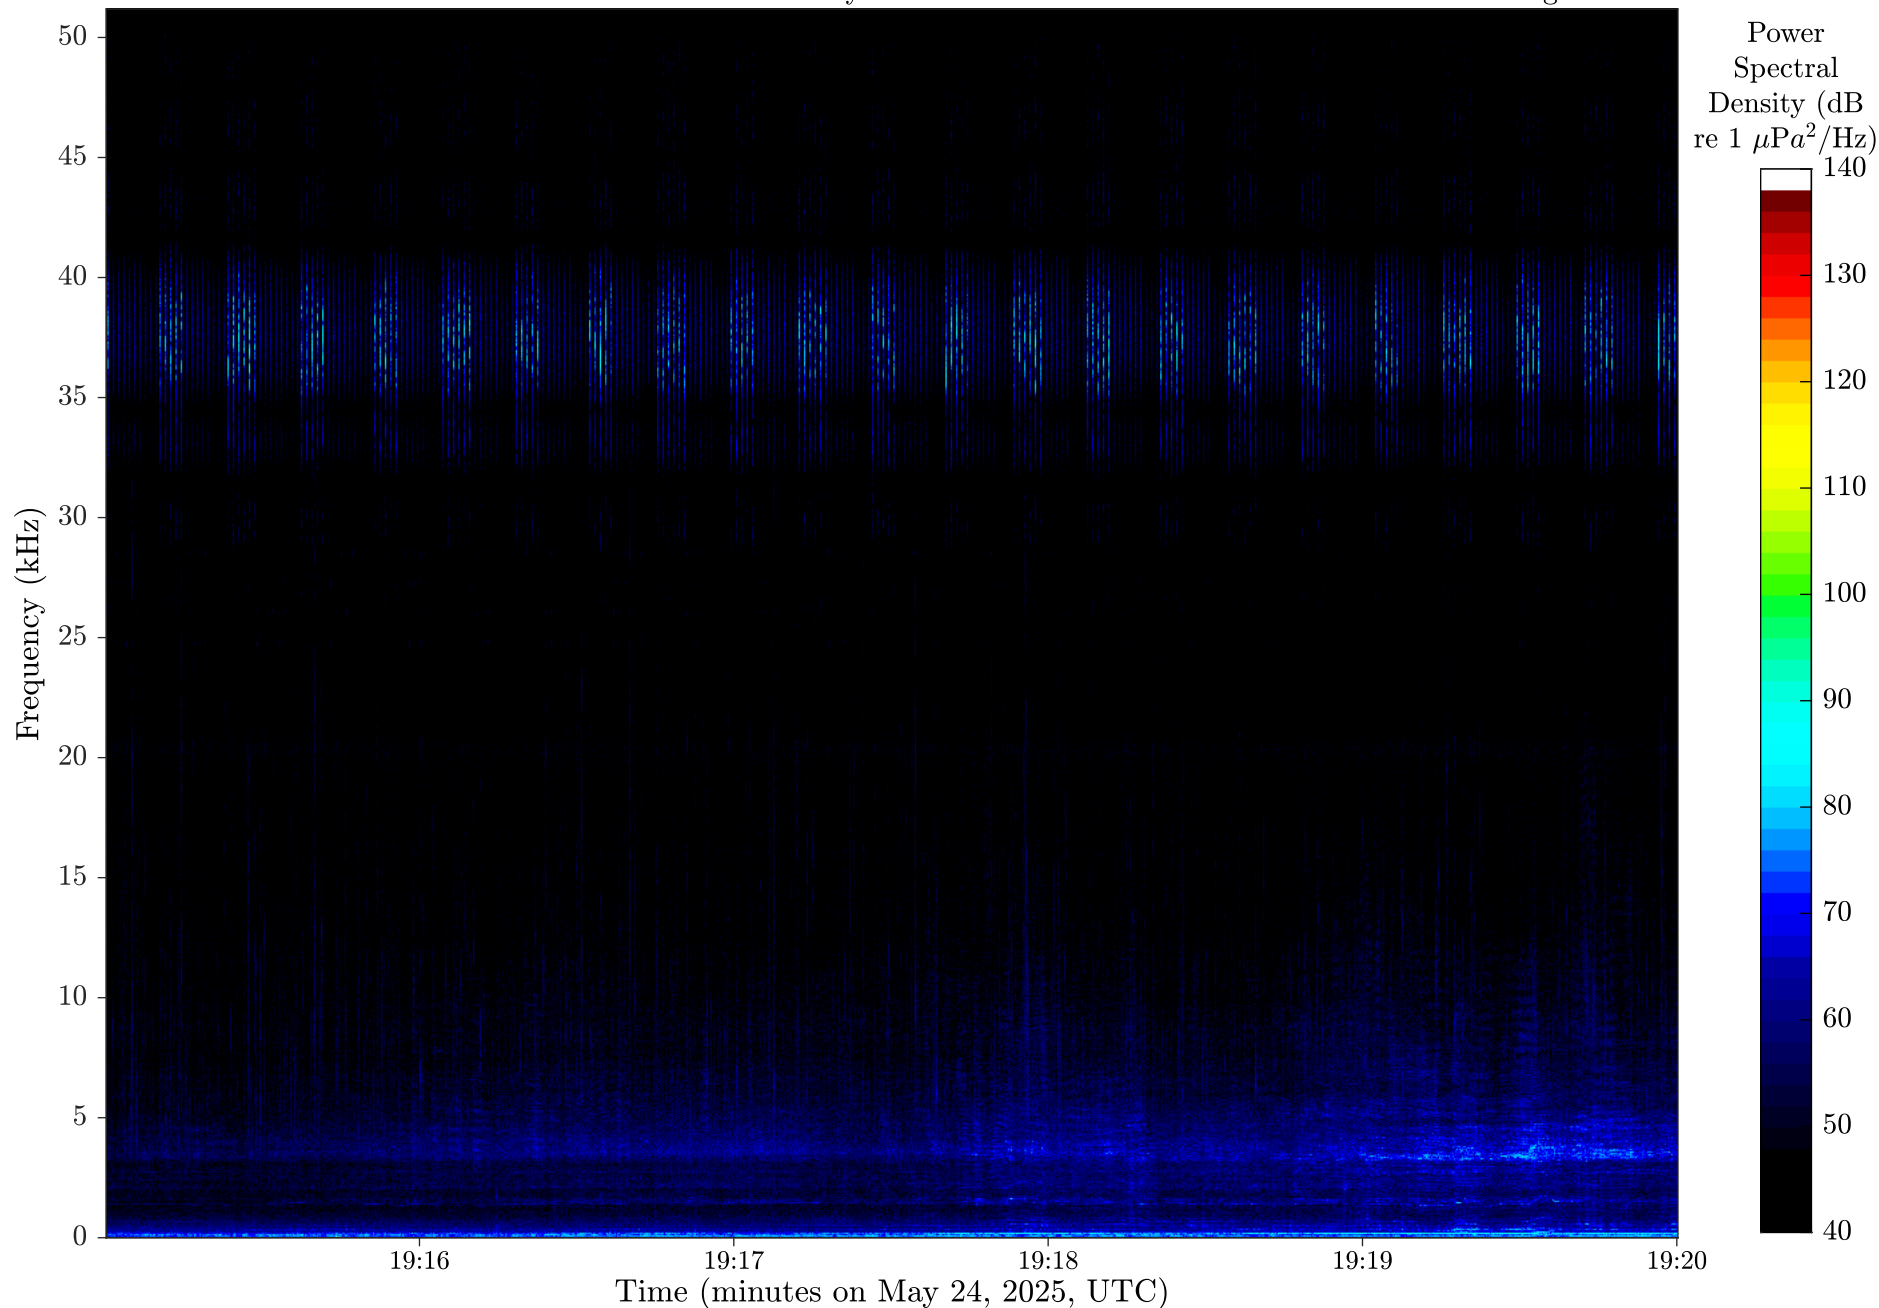


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:47:00 UTC

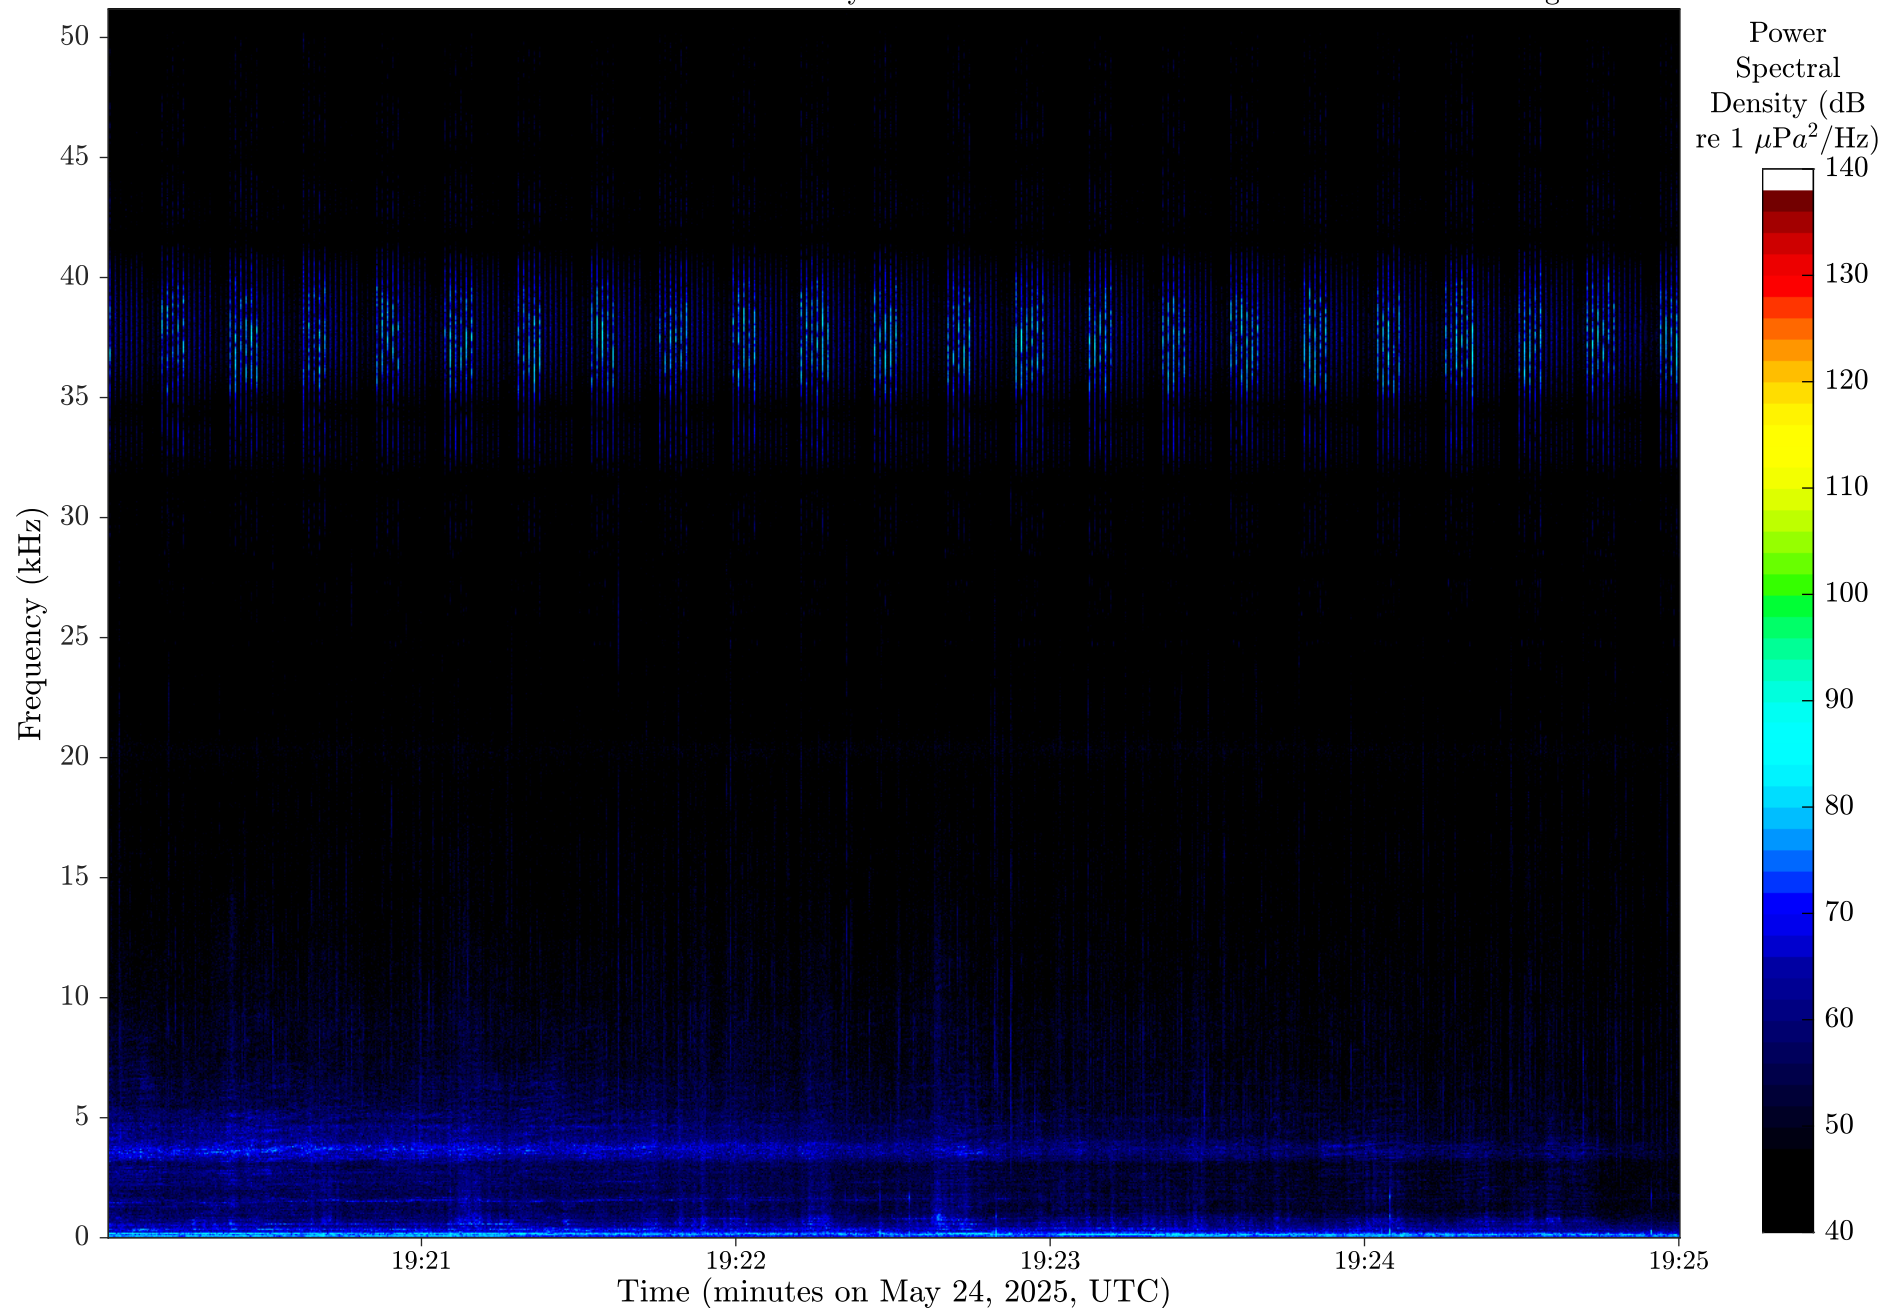

Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:47:08 UTC

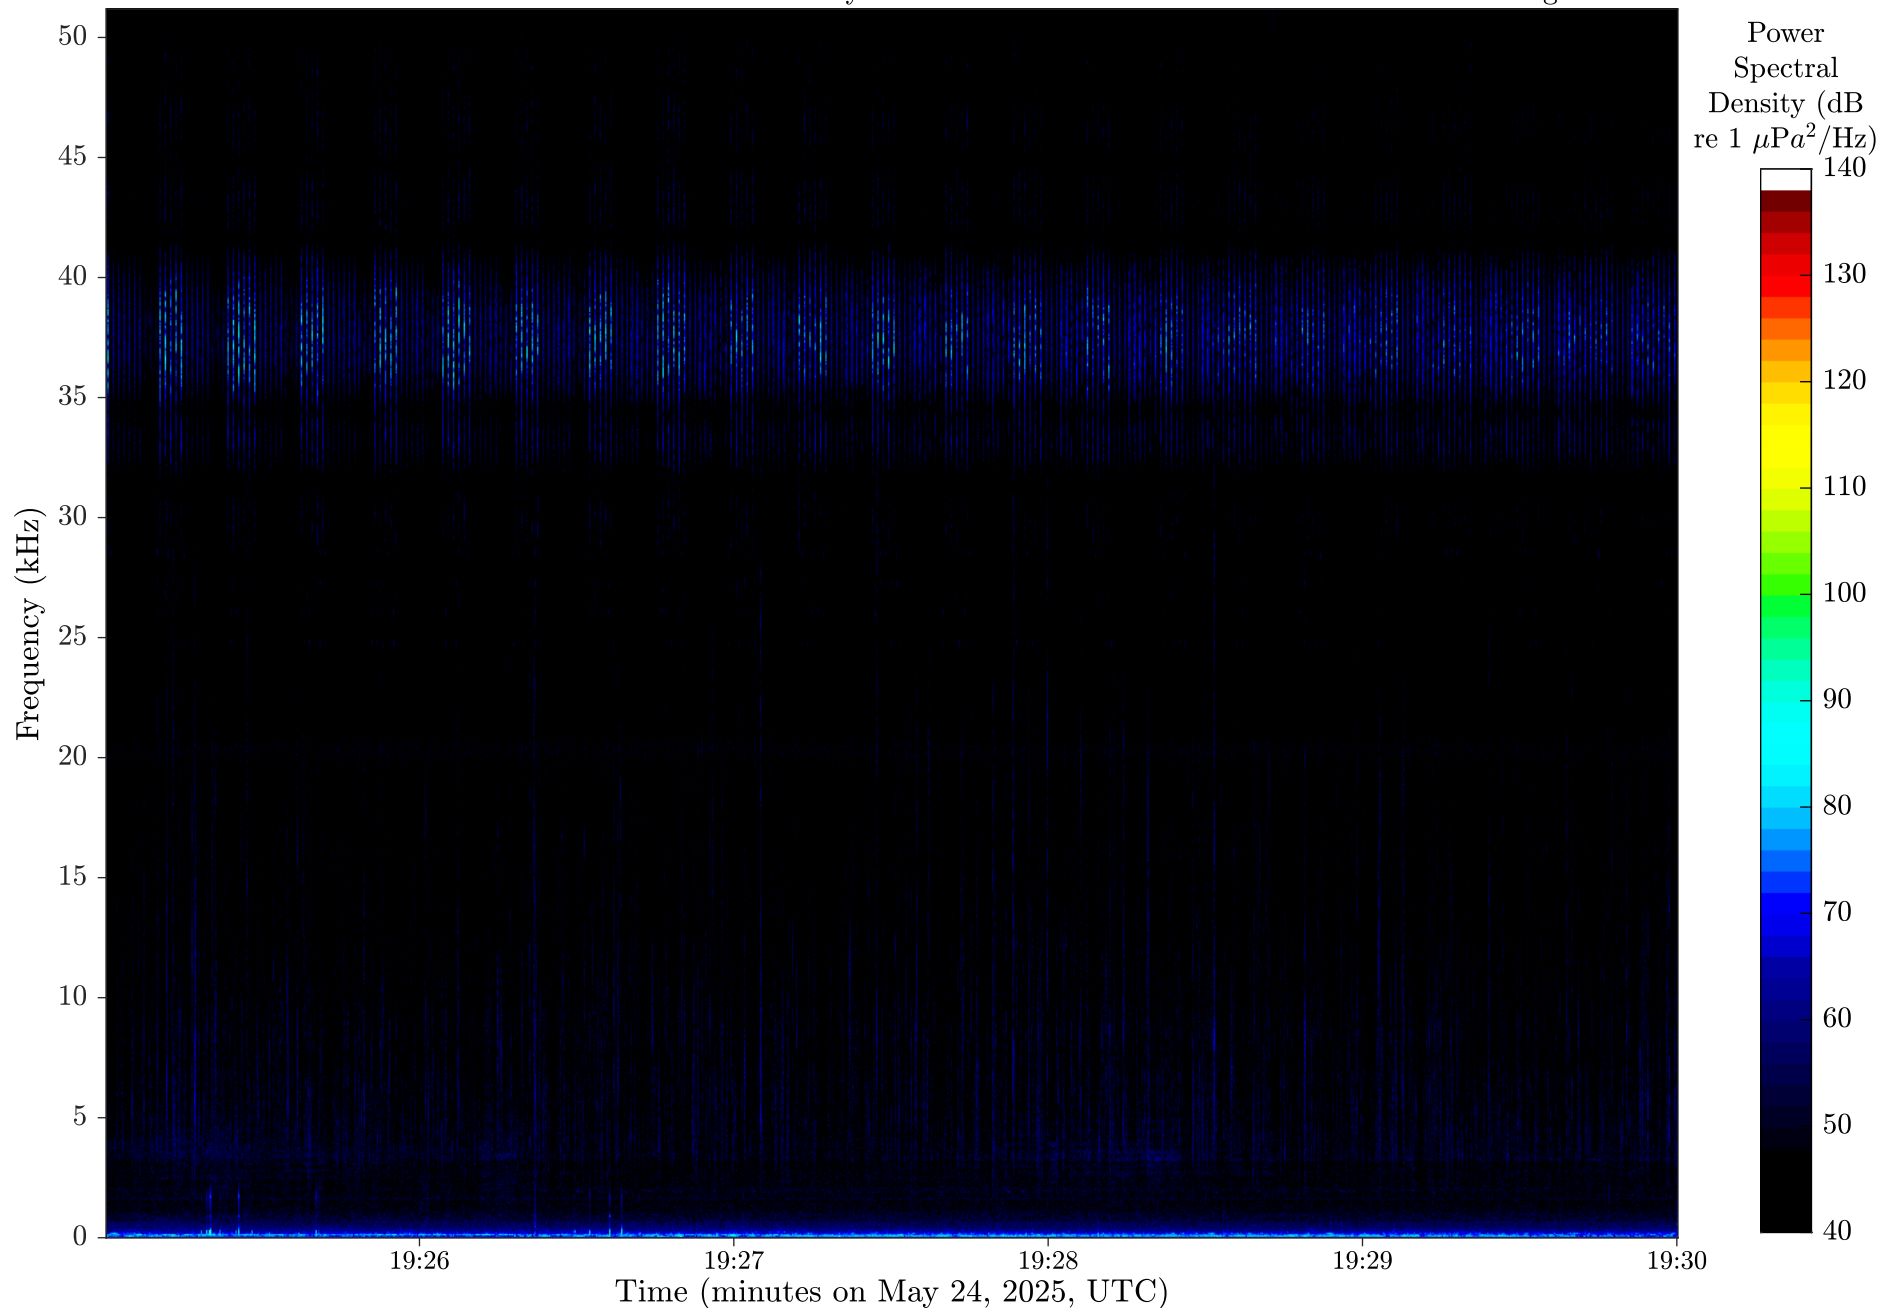

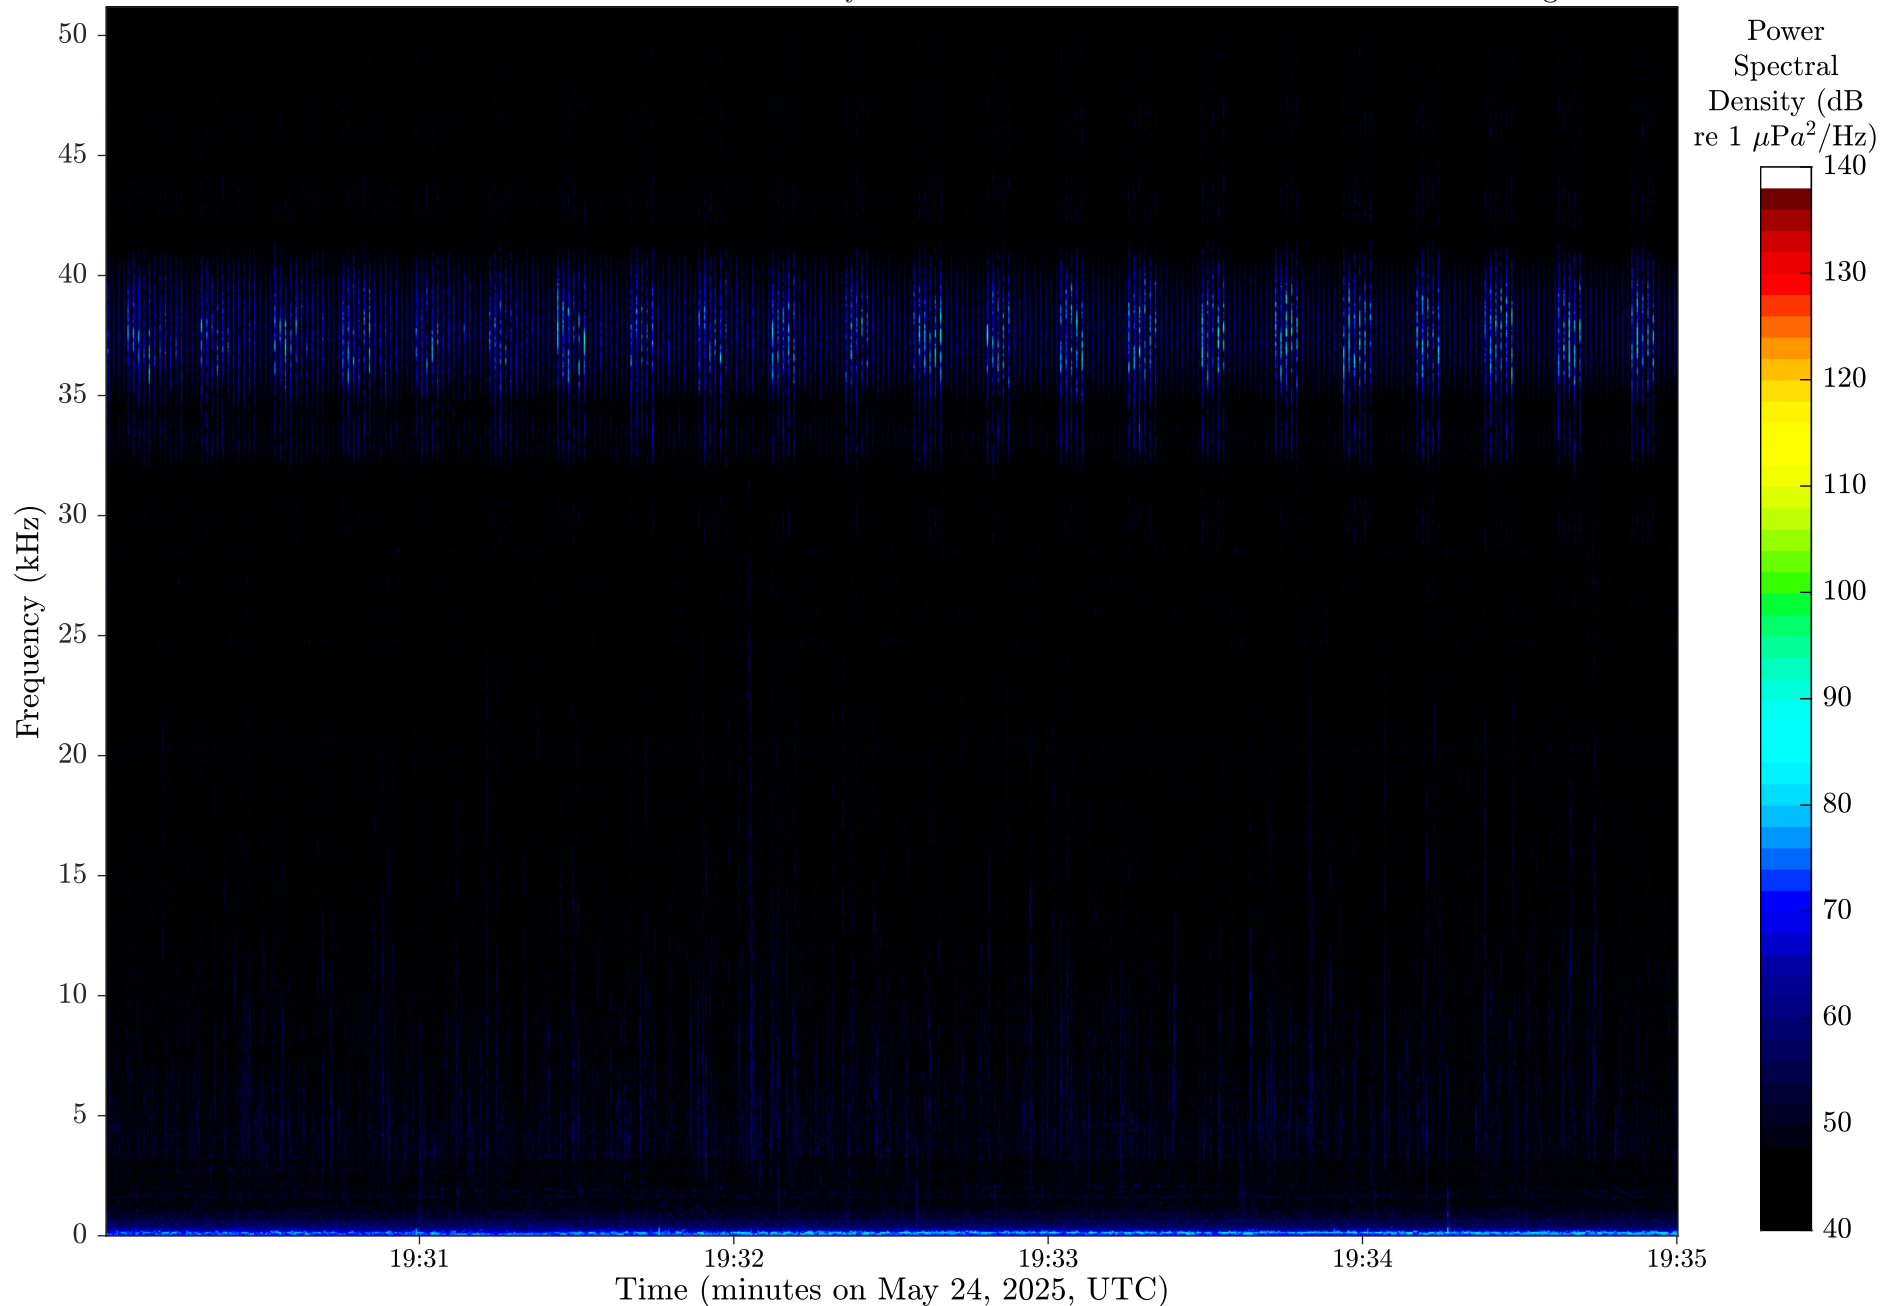


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:47:24 UTC

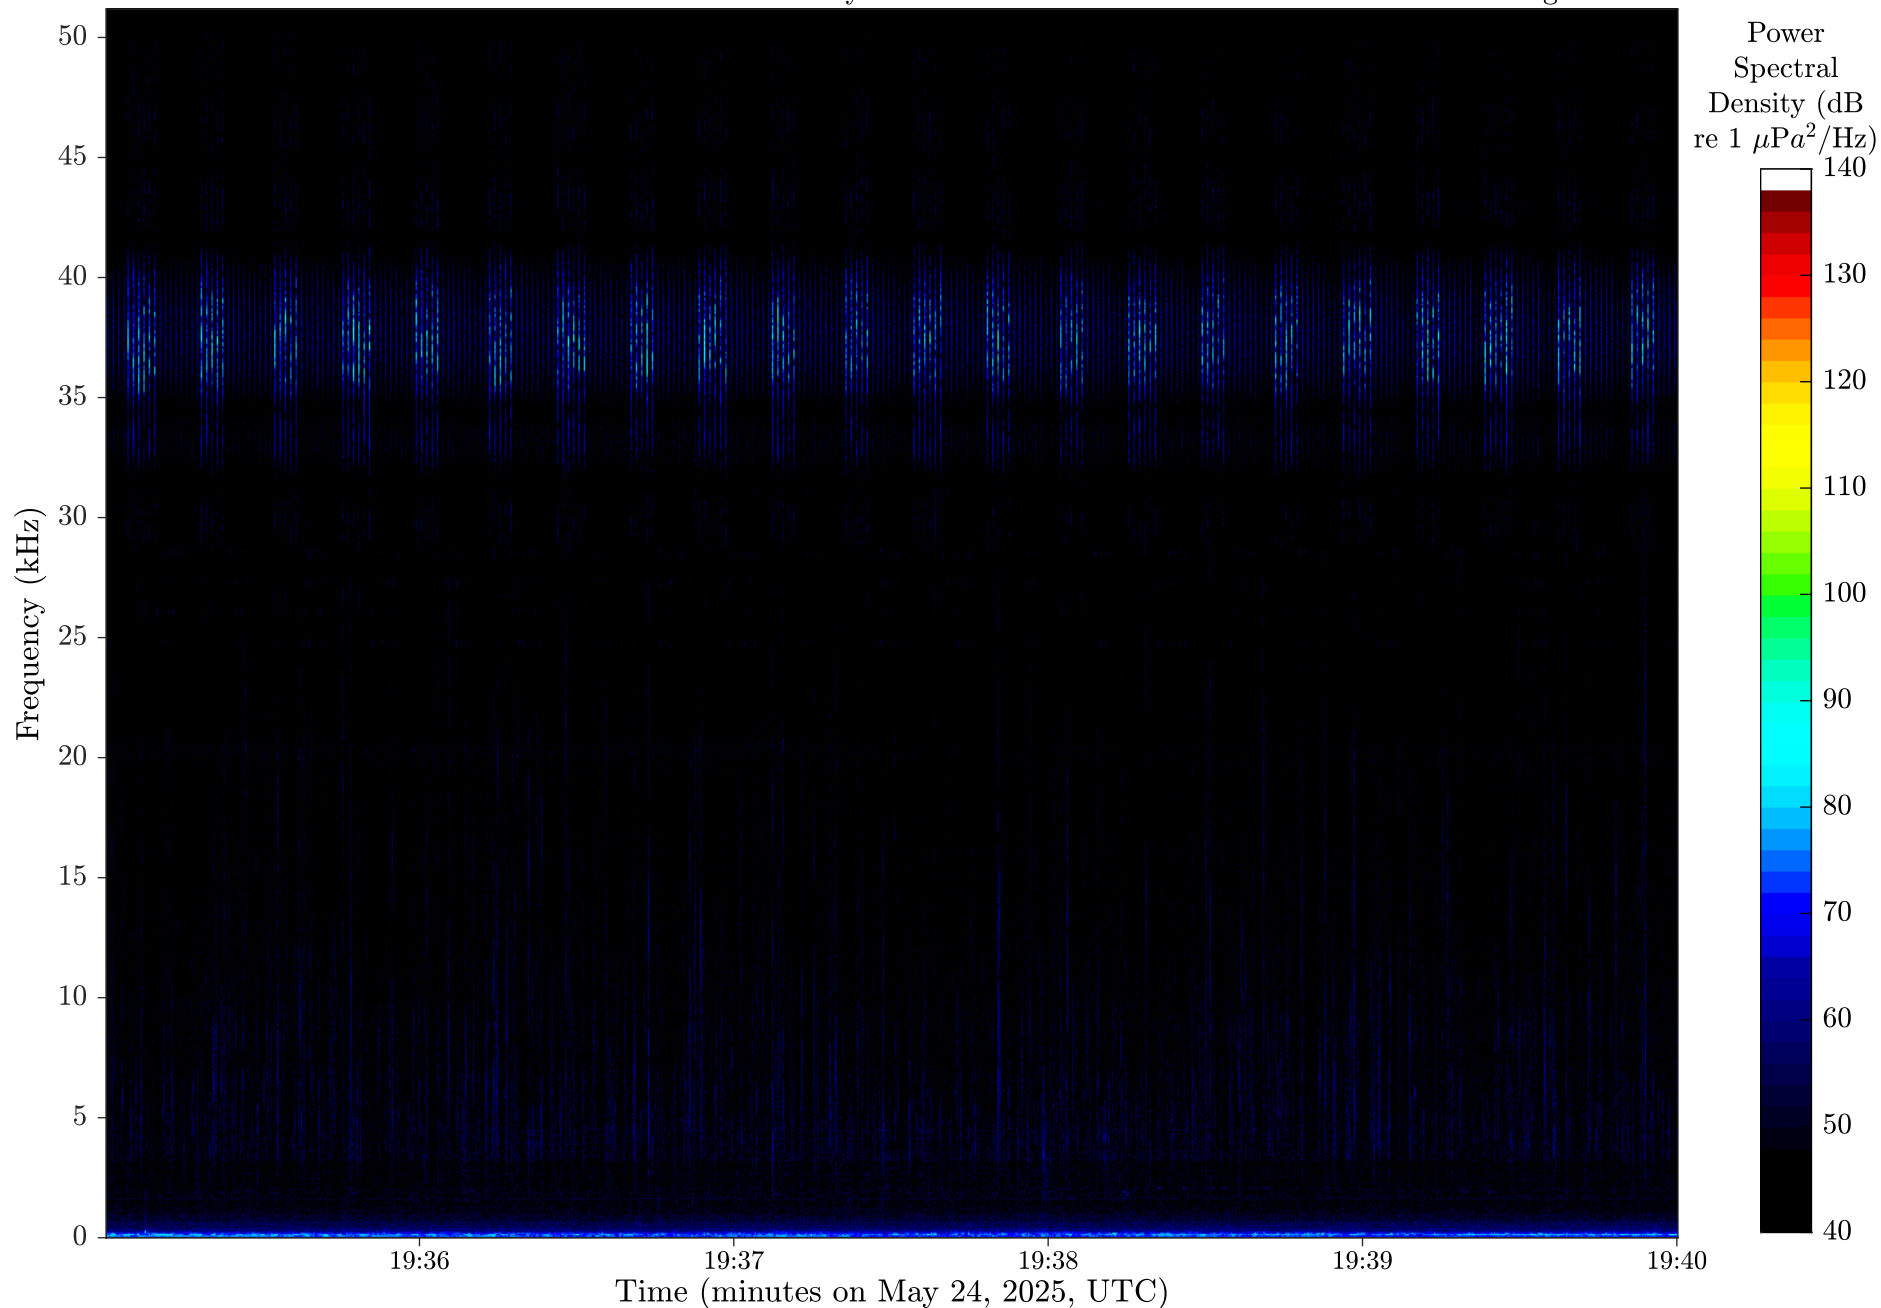


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:47:32 UTC

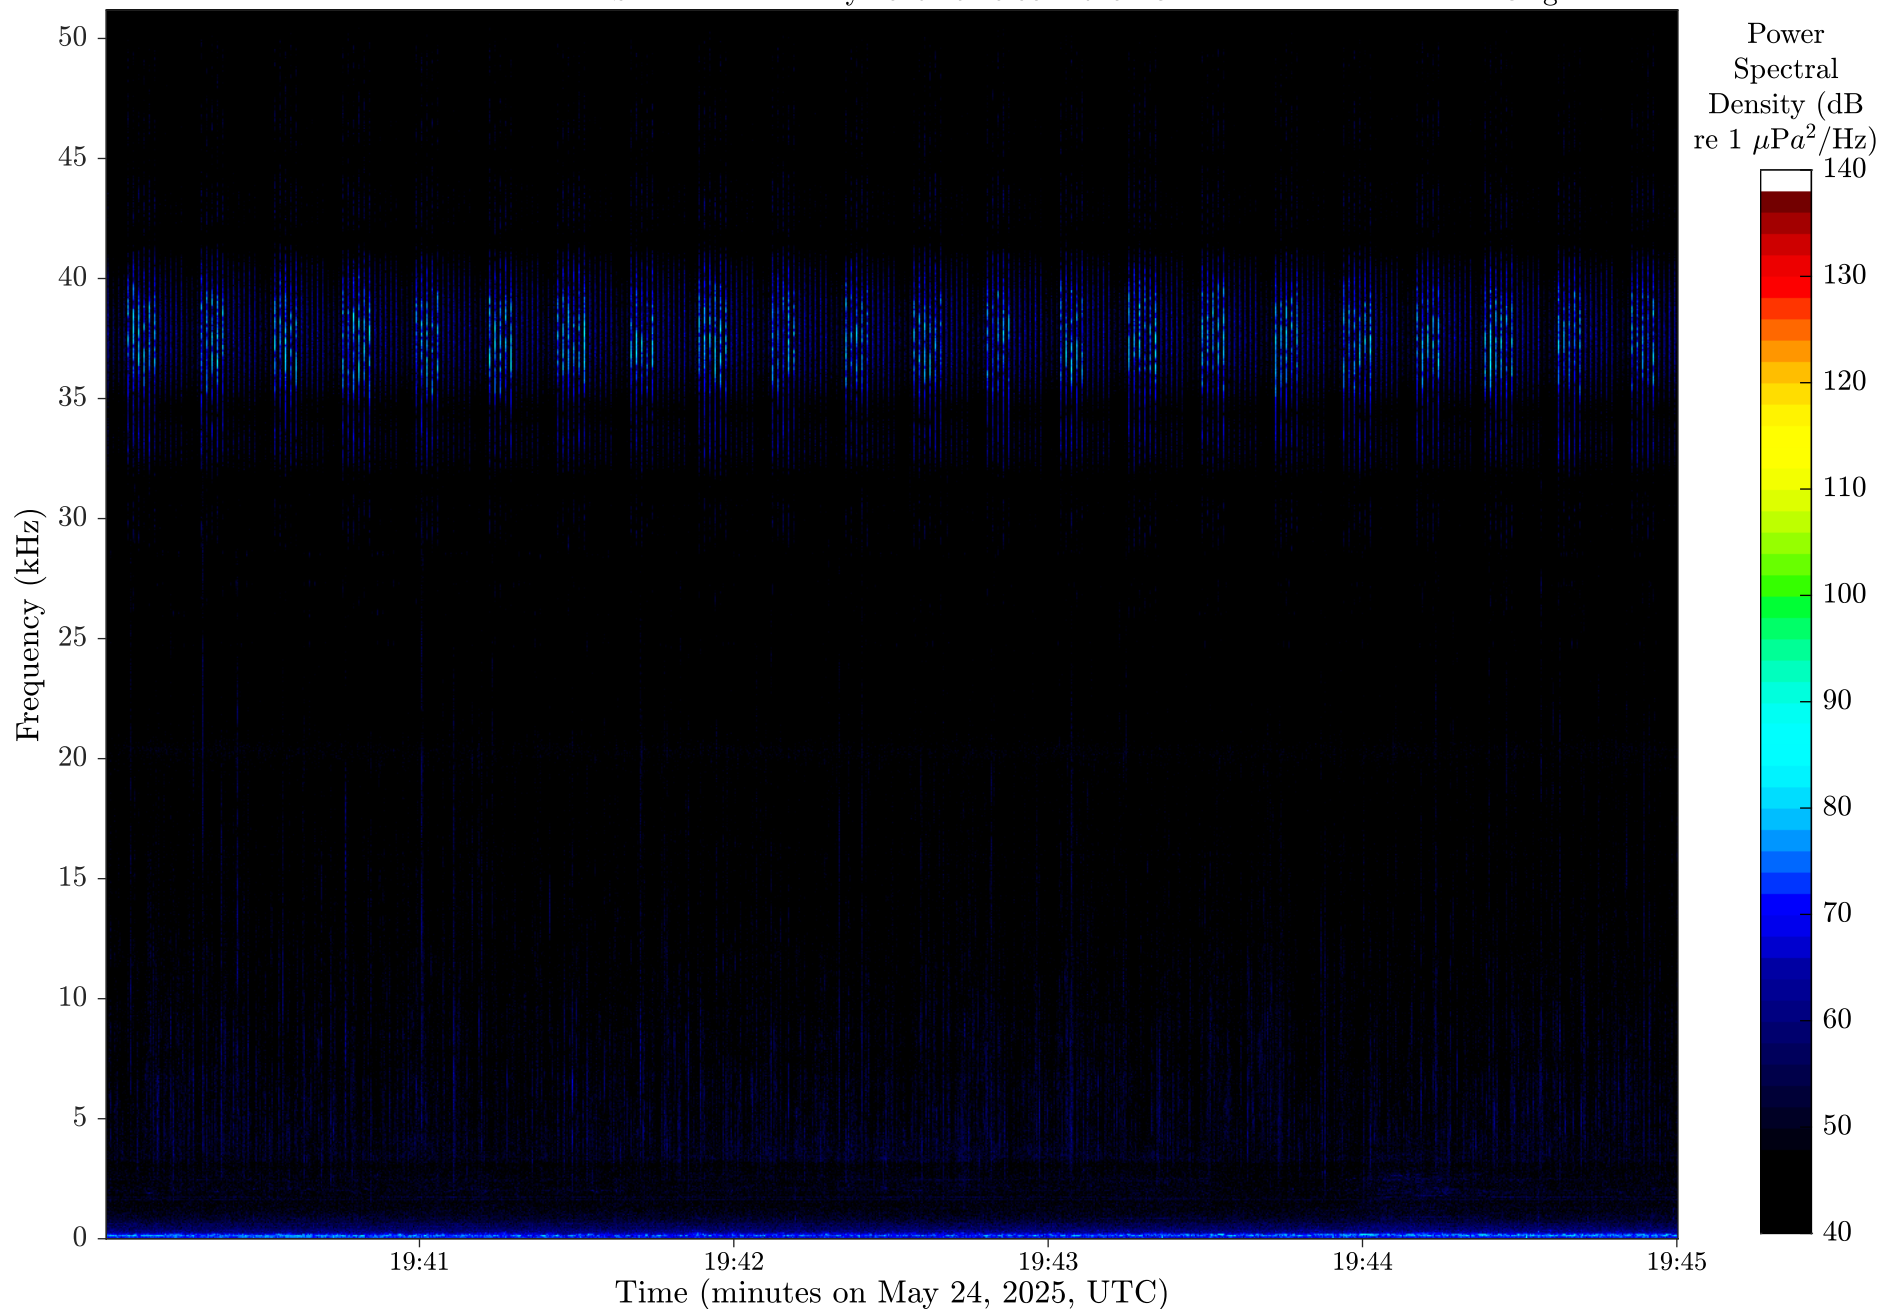


Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:47:41 UTC

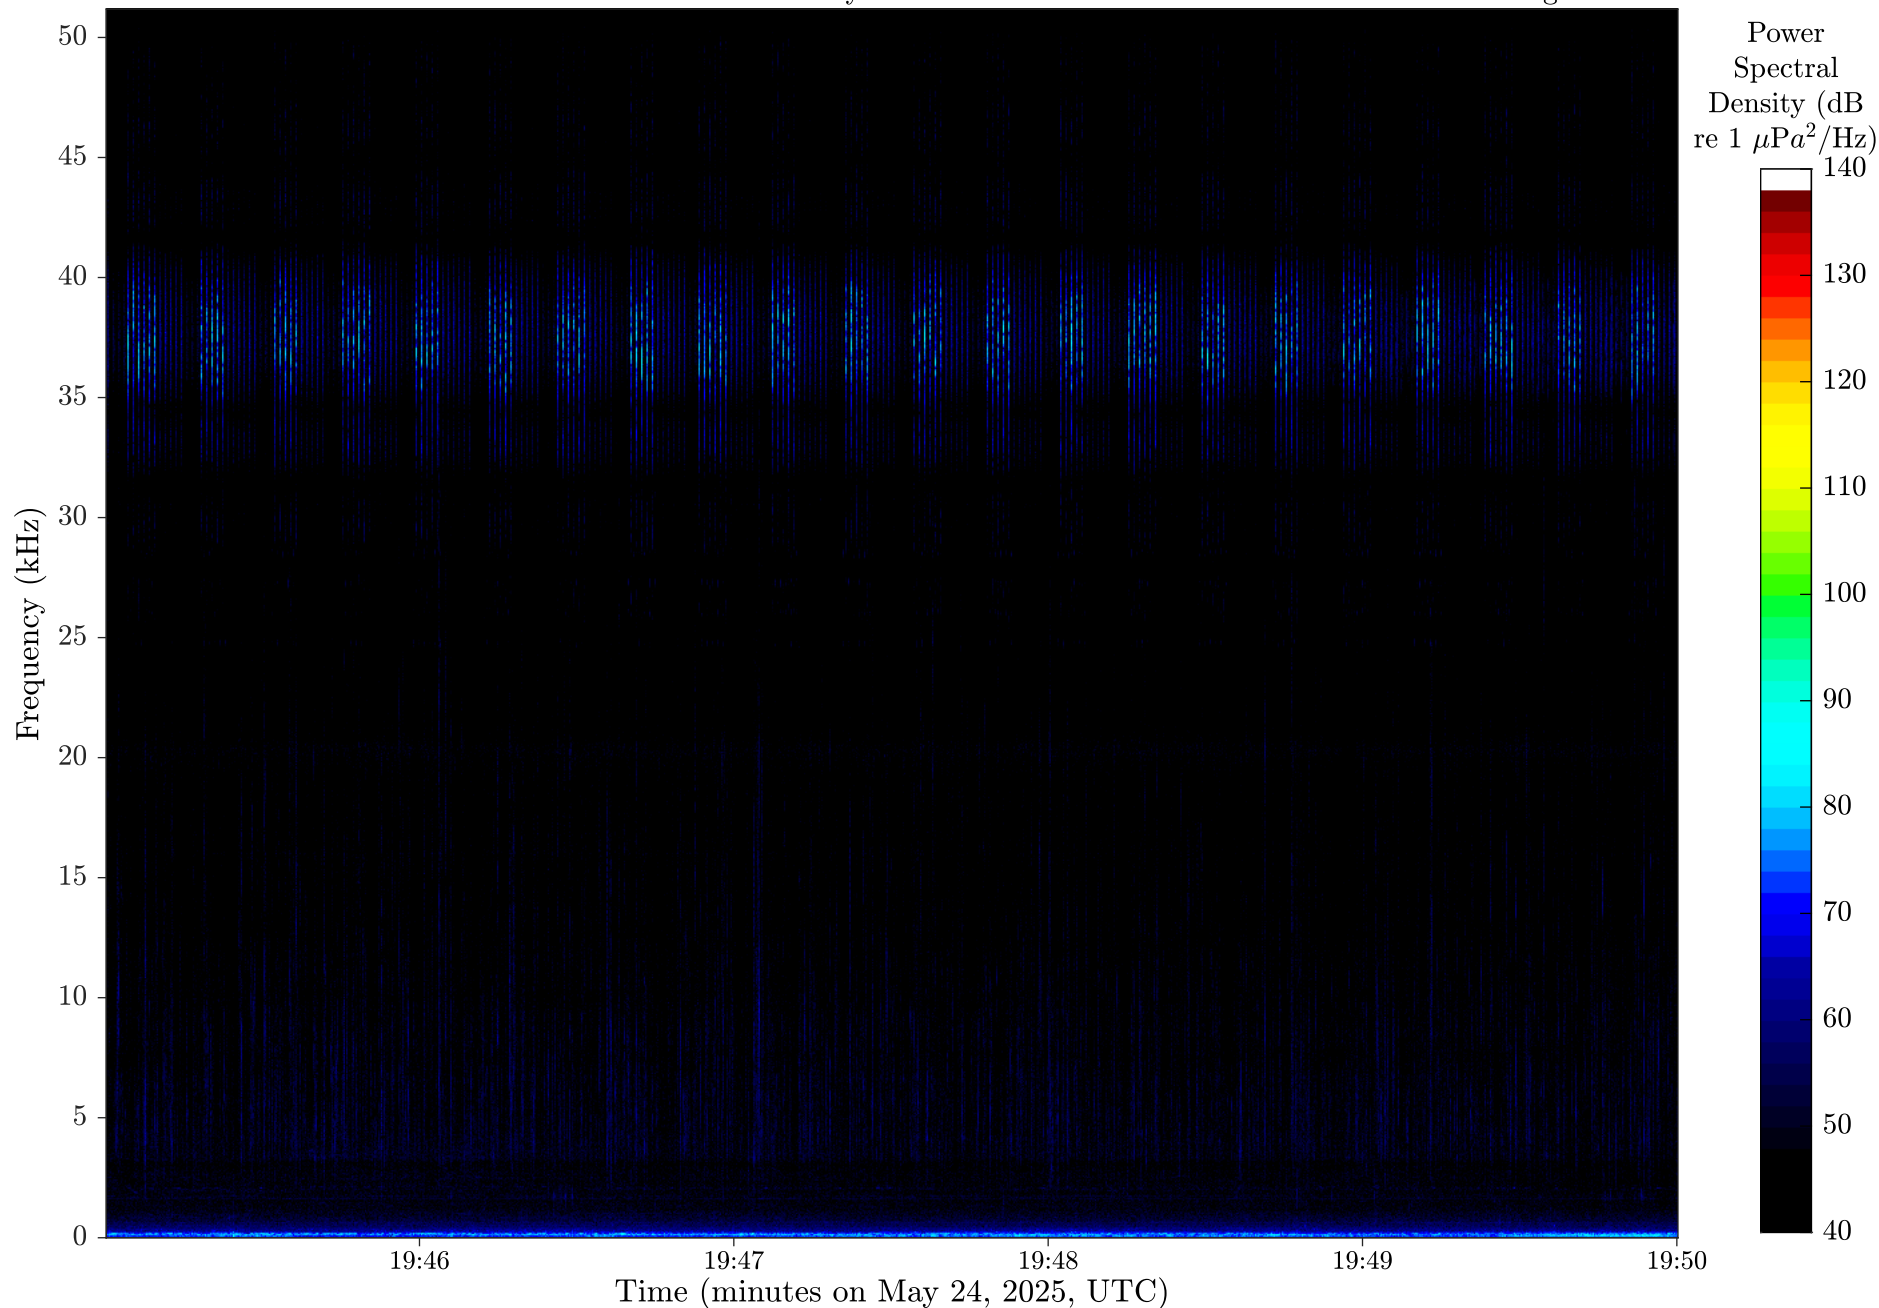


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:47:49 UTC

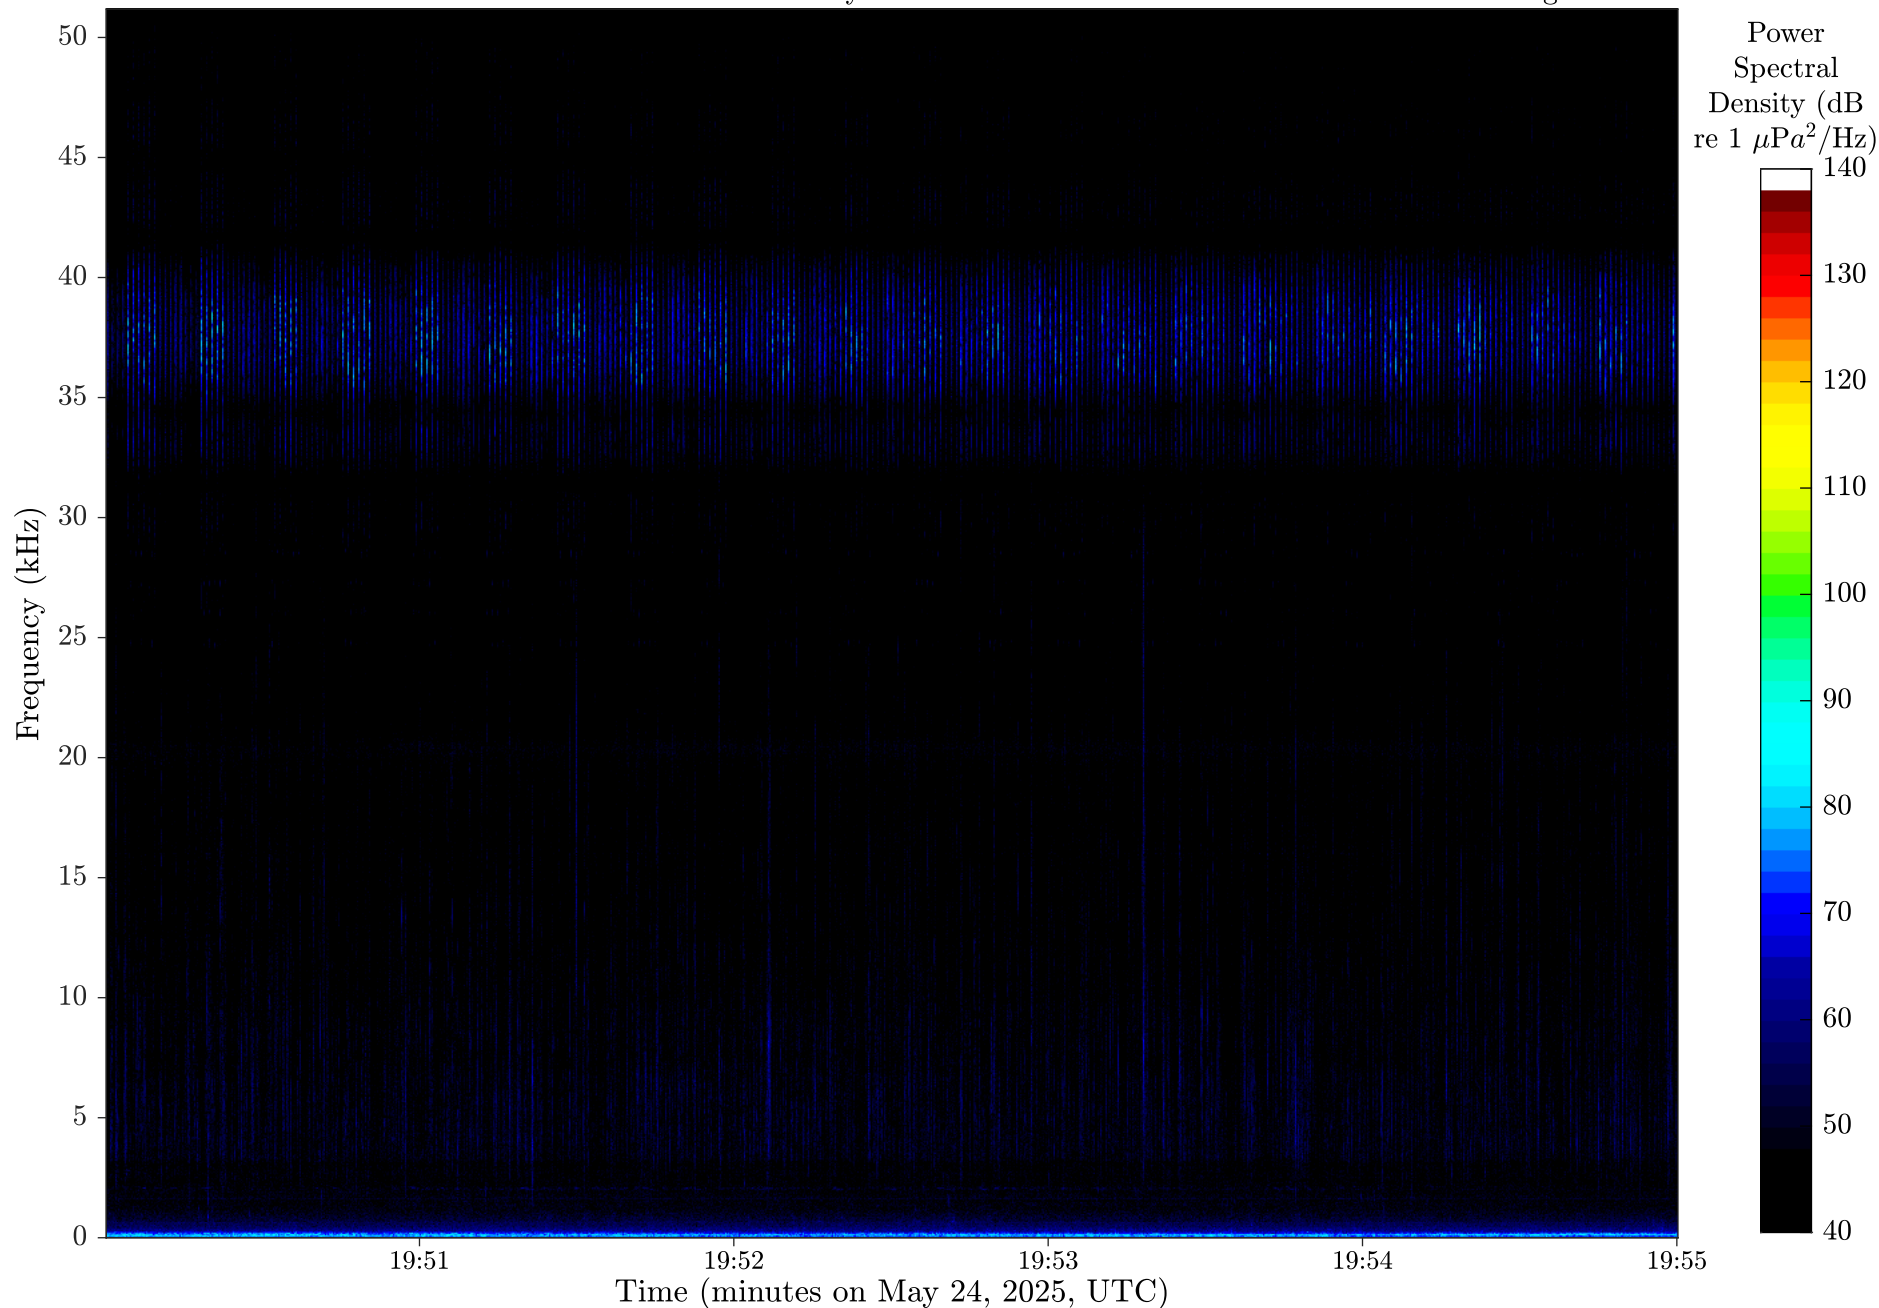


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:47:58 UTC

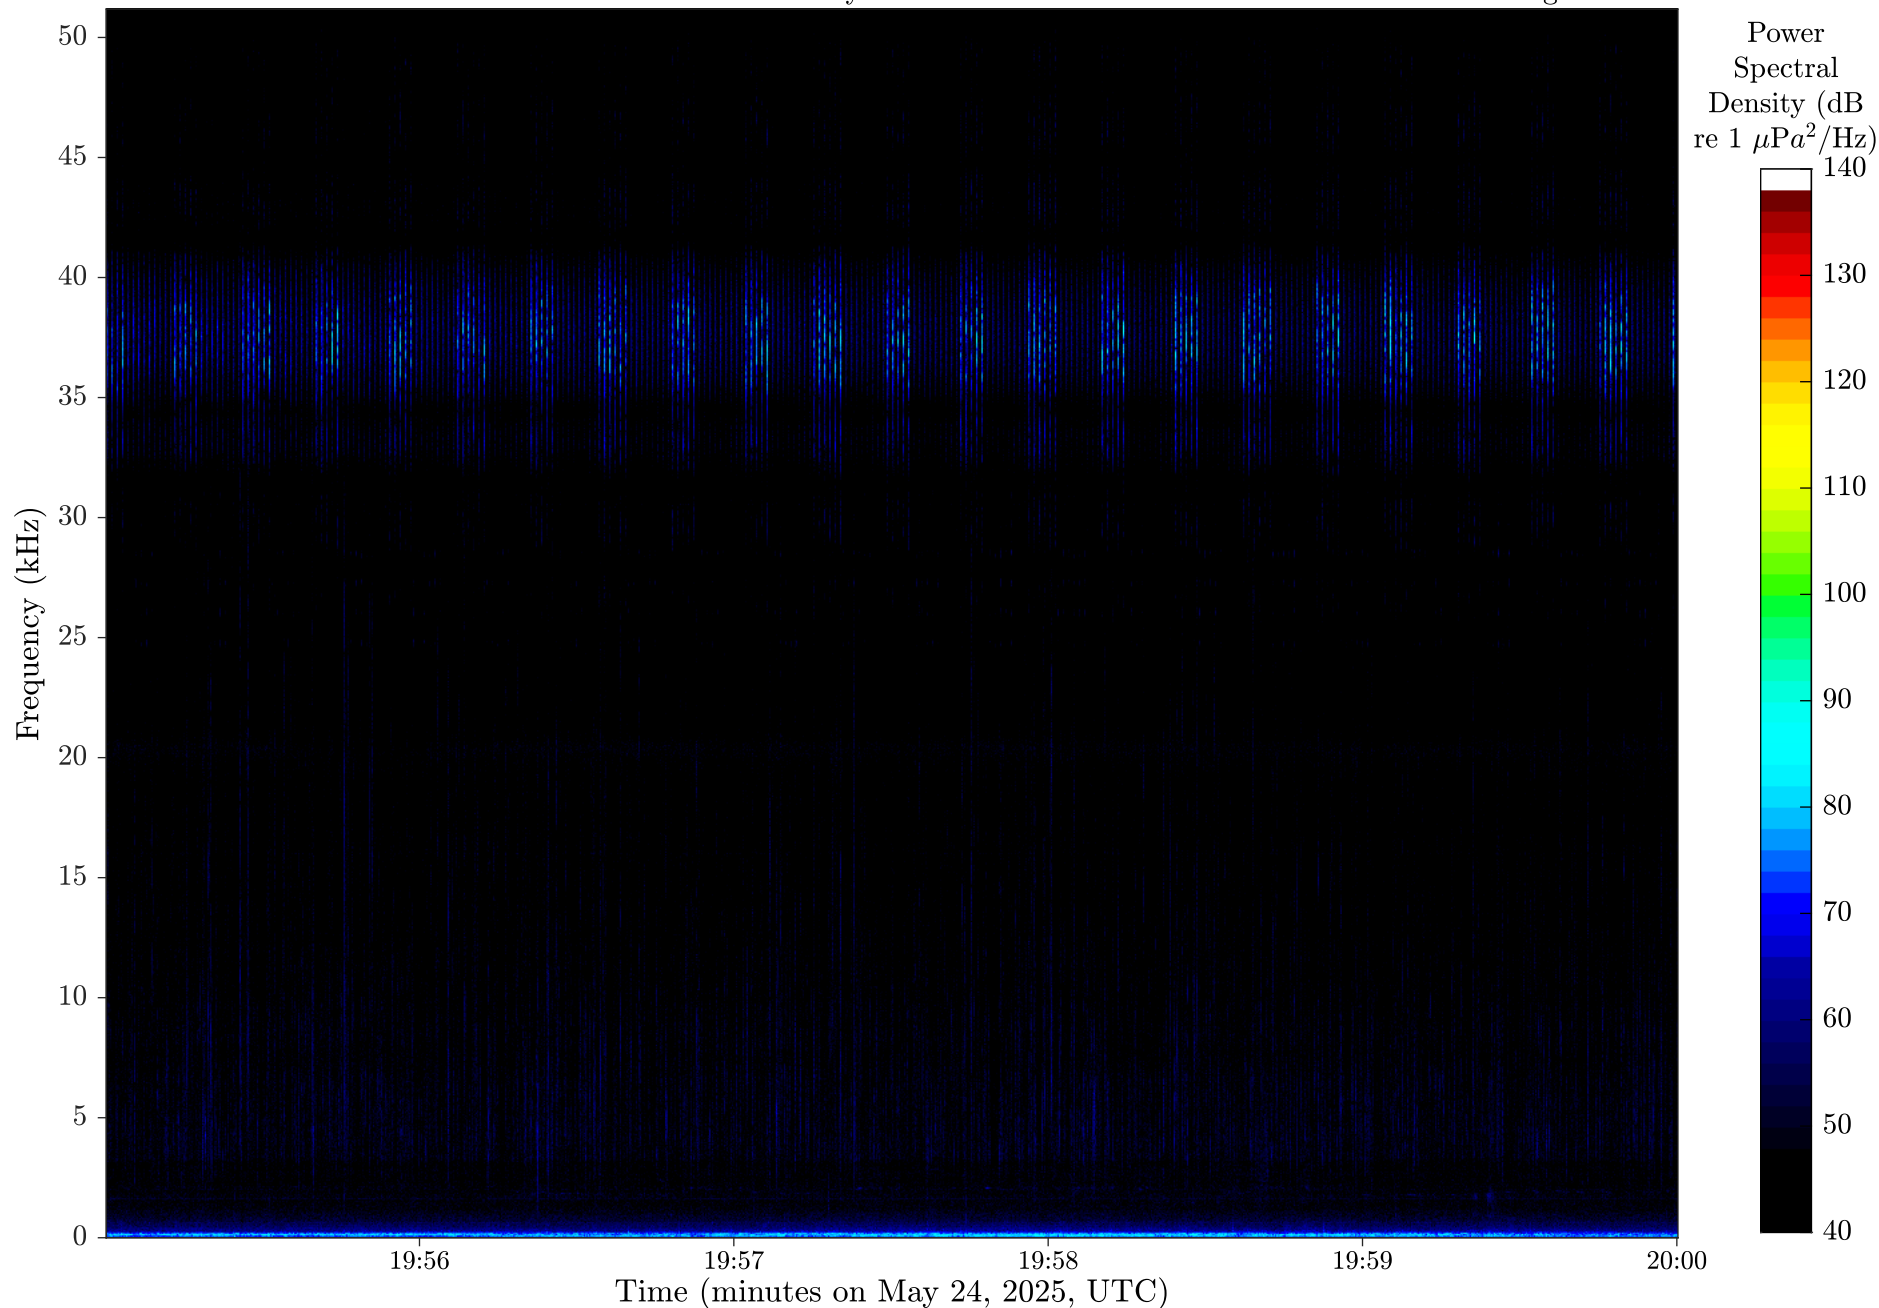


Comments: 34.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:48:06 UTC

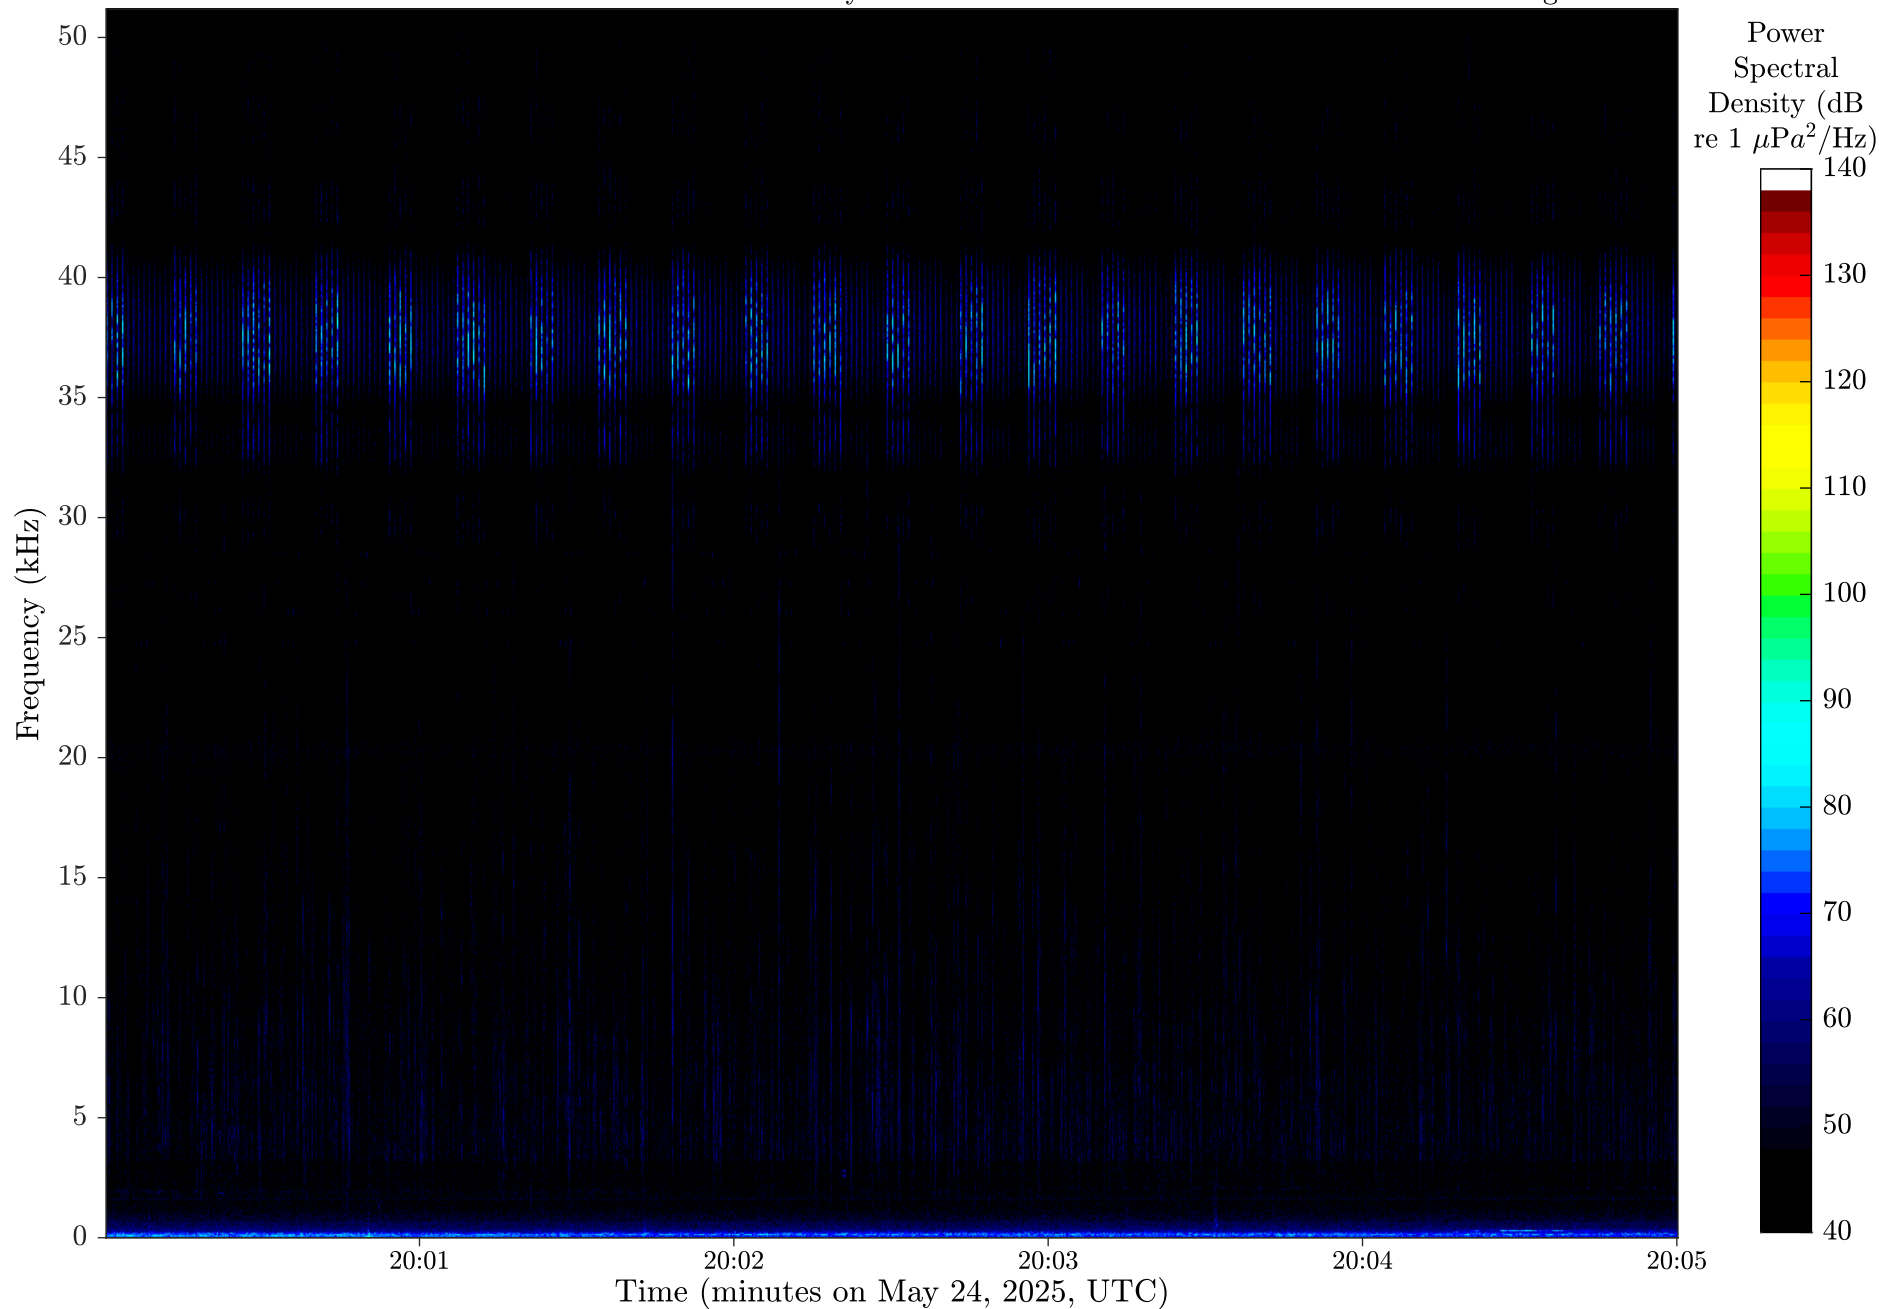


Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:48:14 UTC

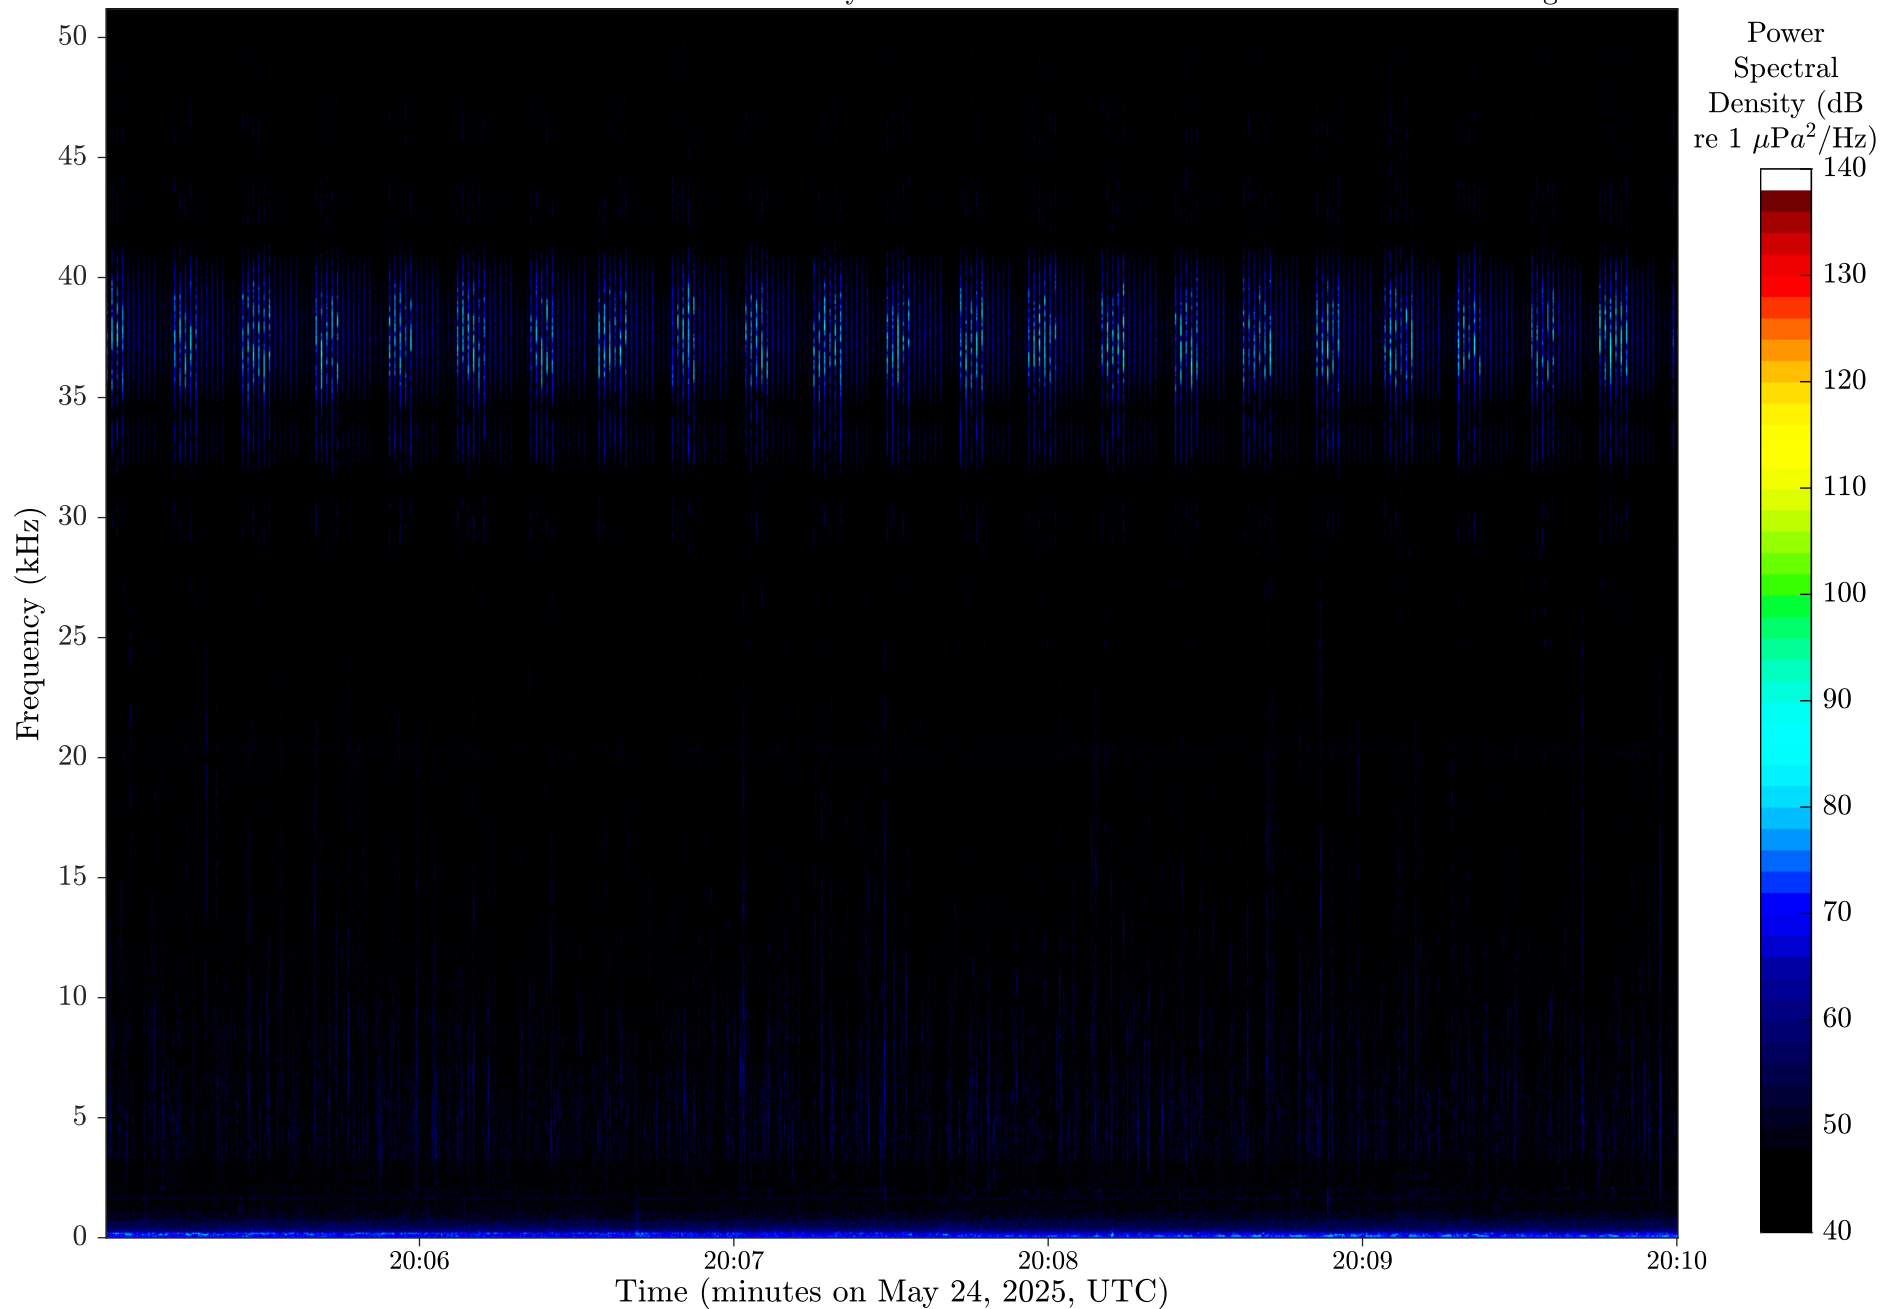

Comments: 35.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:48:23 UTC

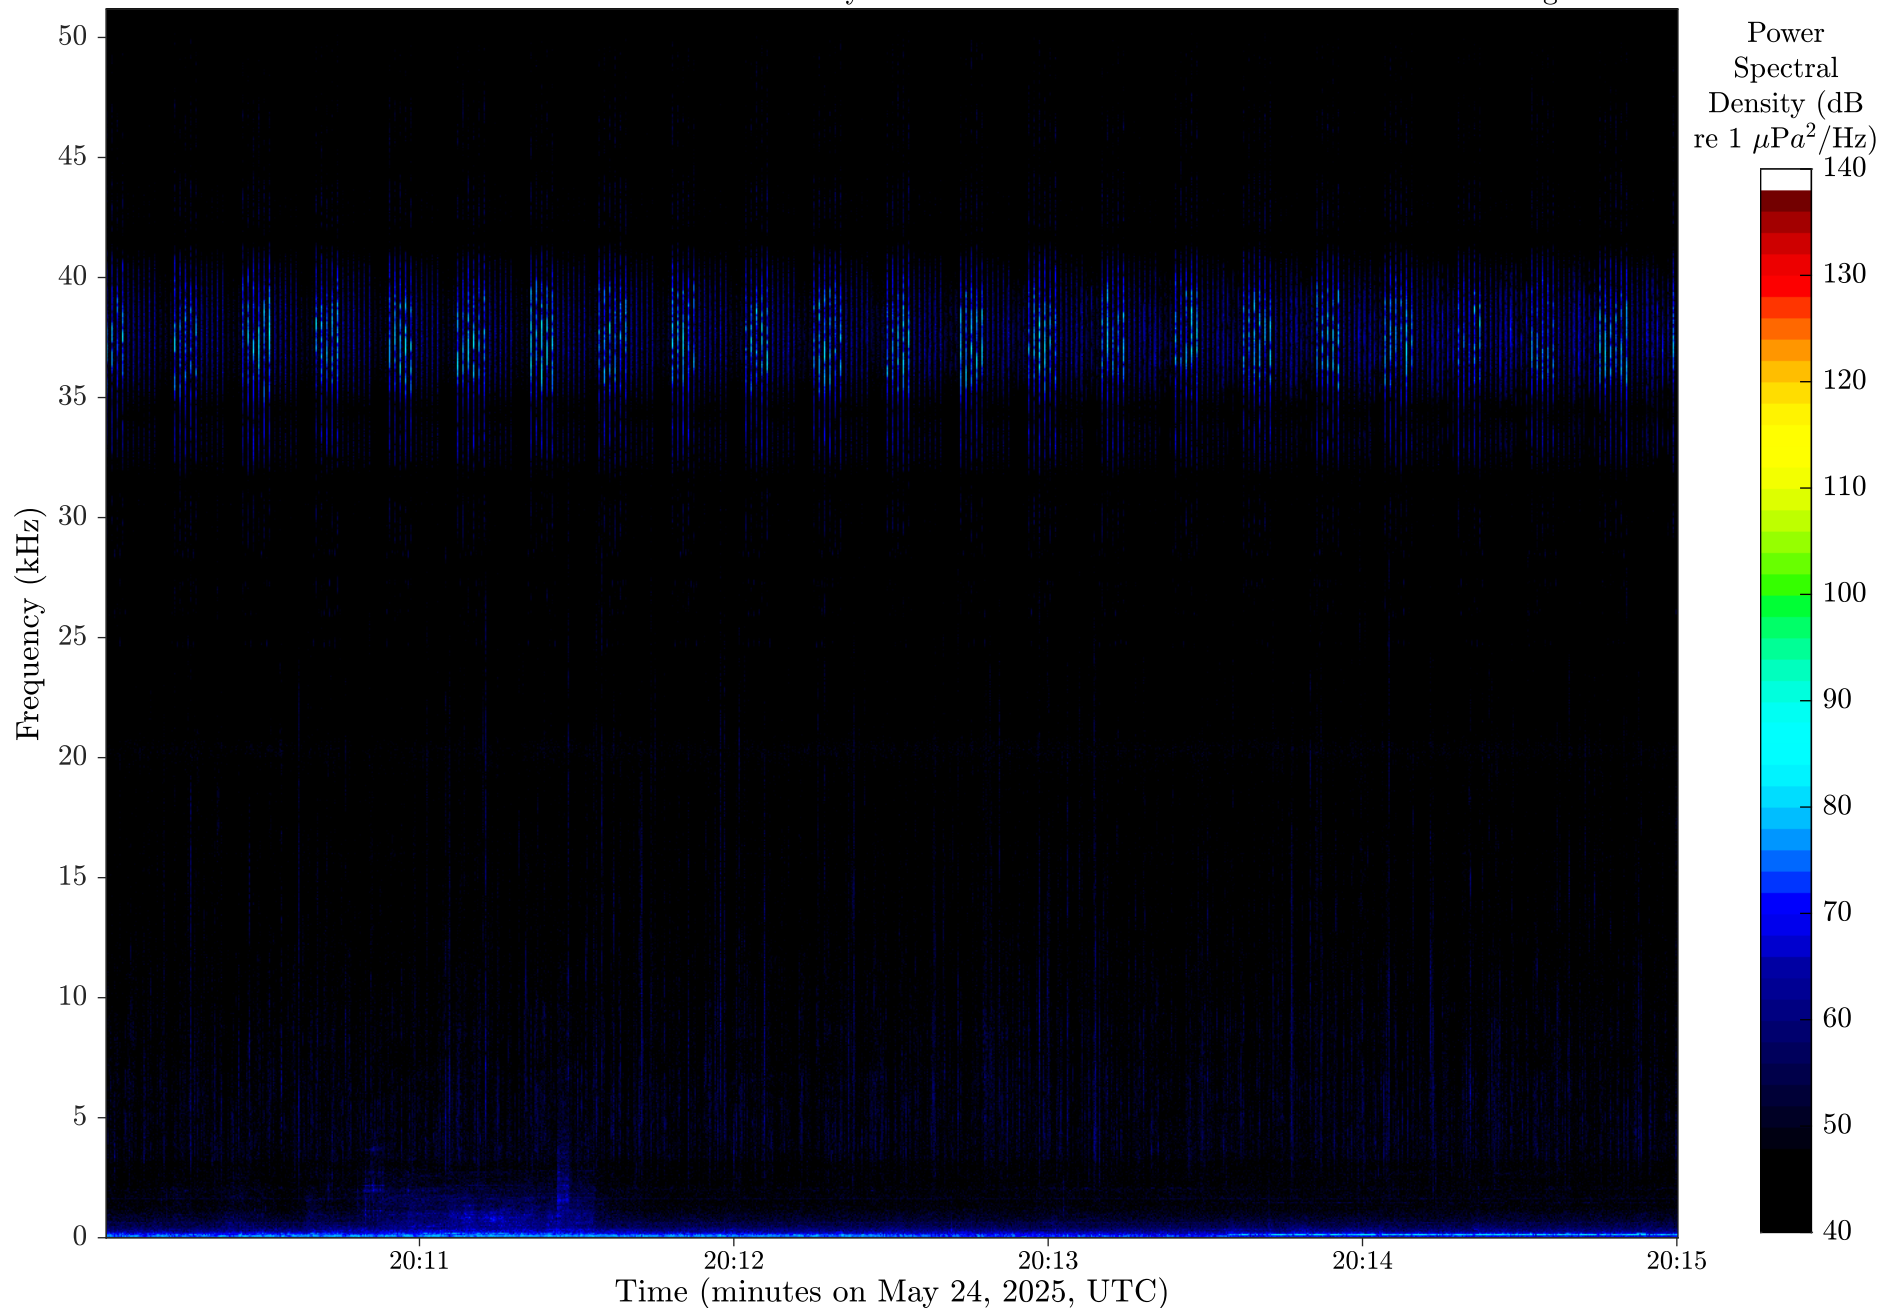

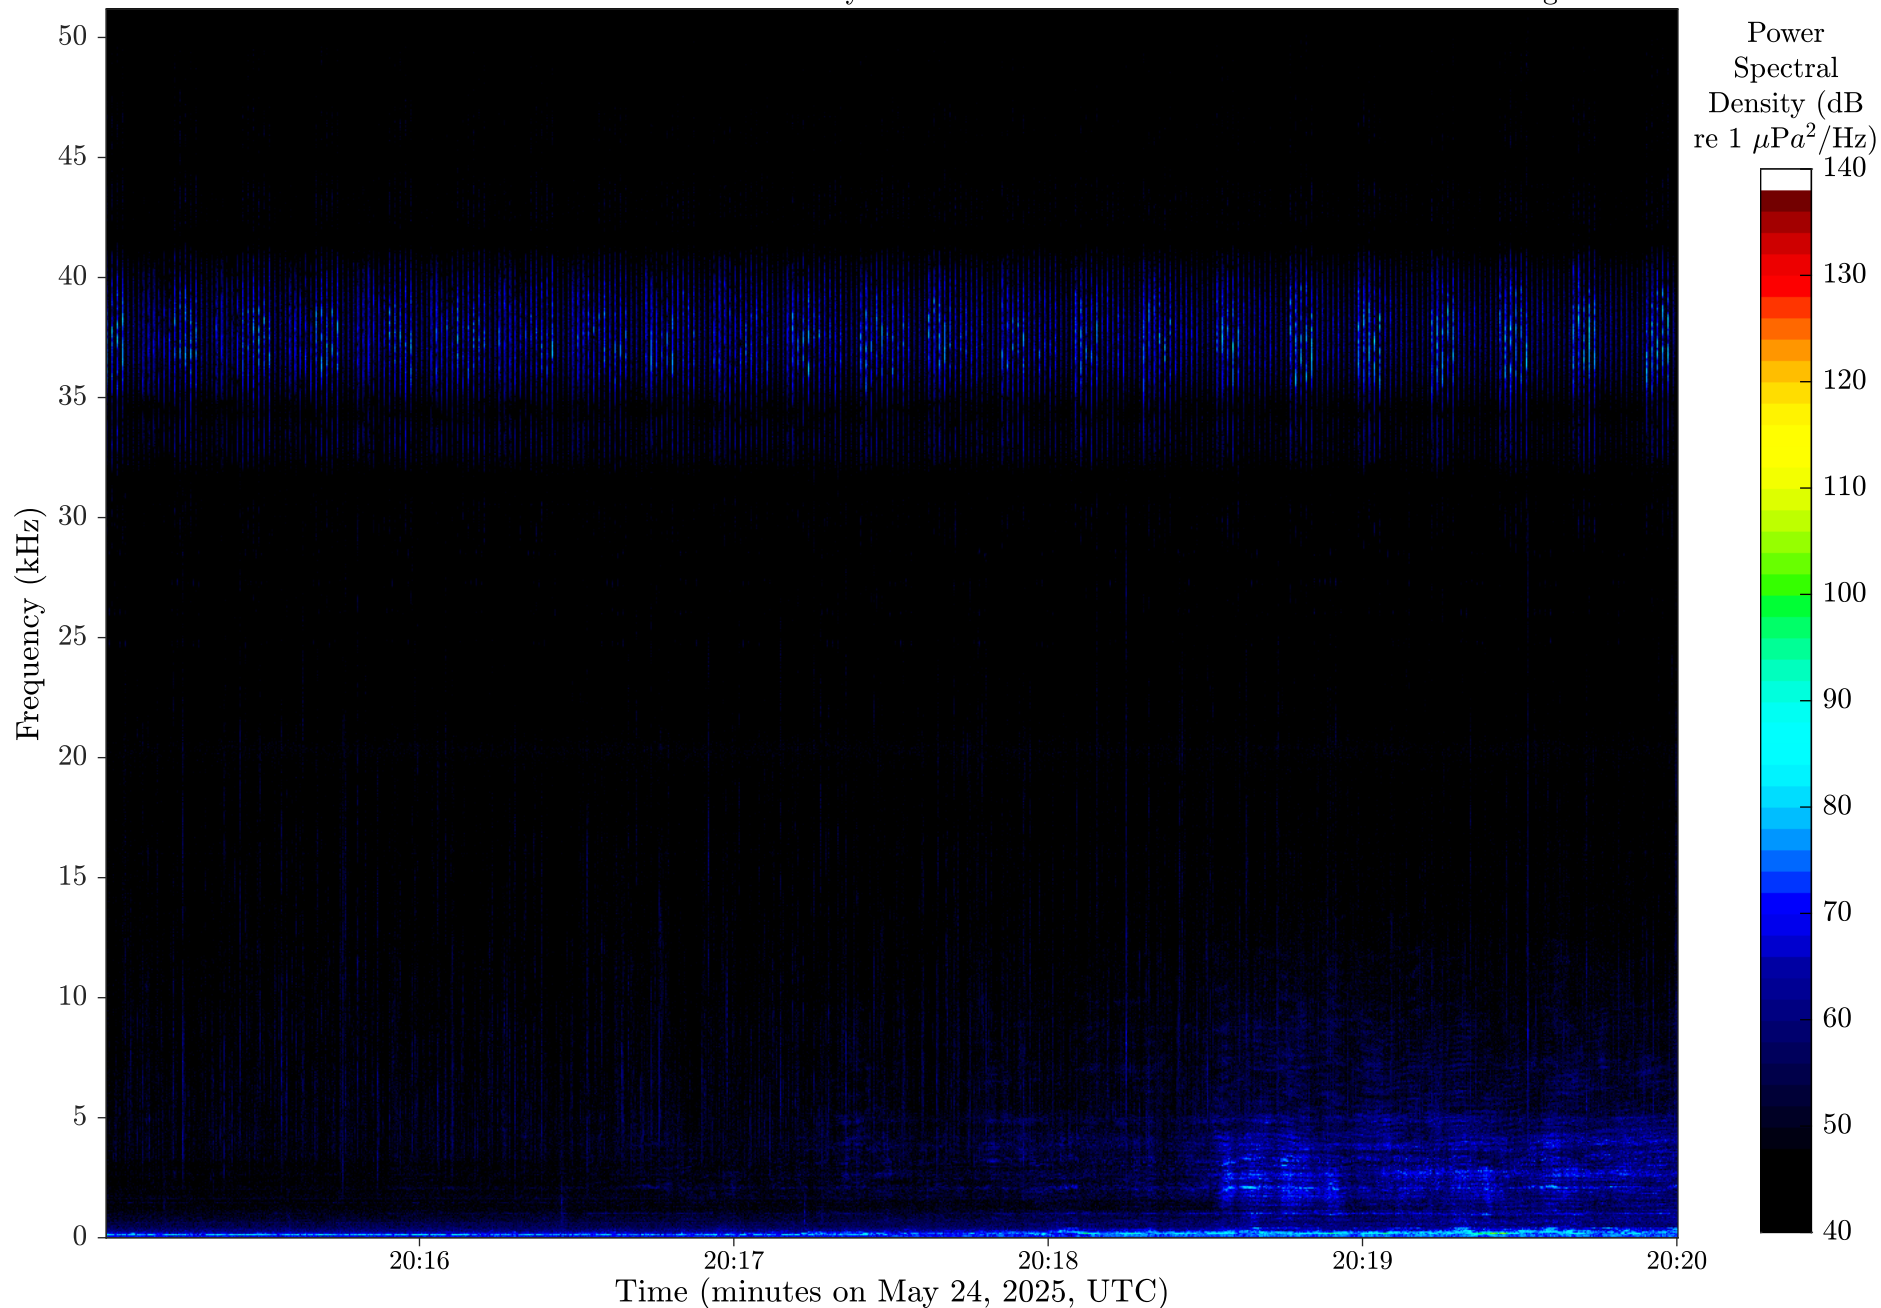


Comments: 33.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:48:39 UTC

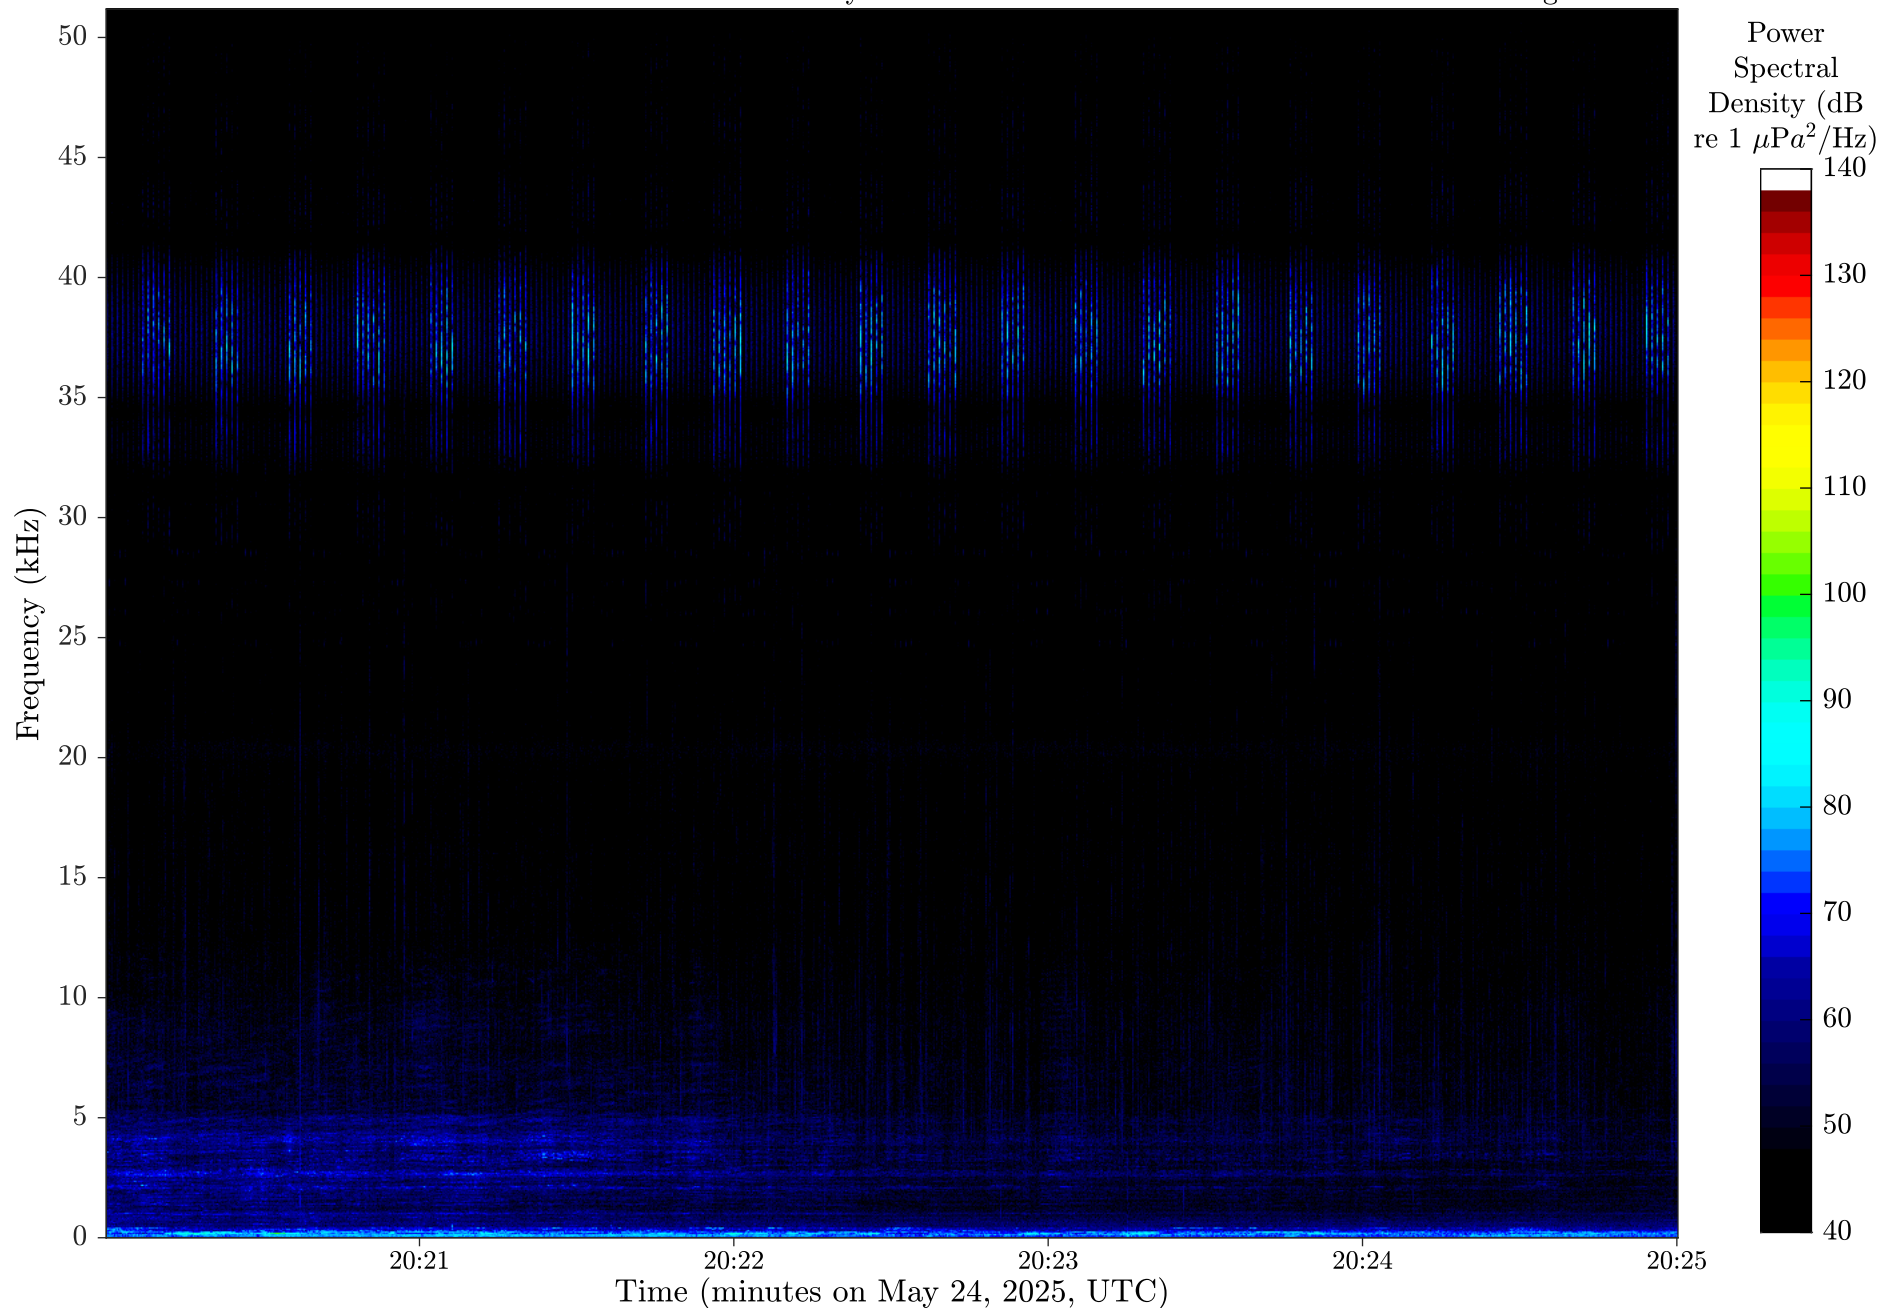


Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:48:47 UTC

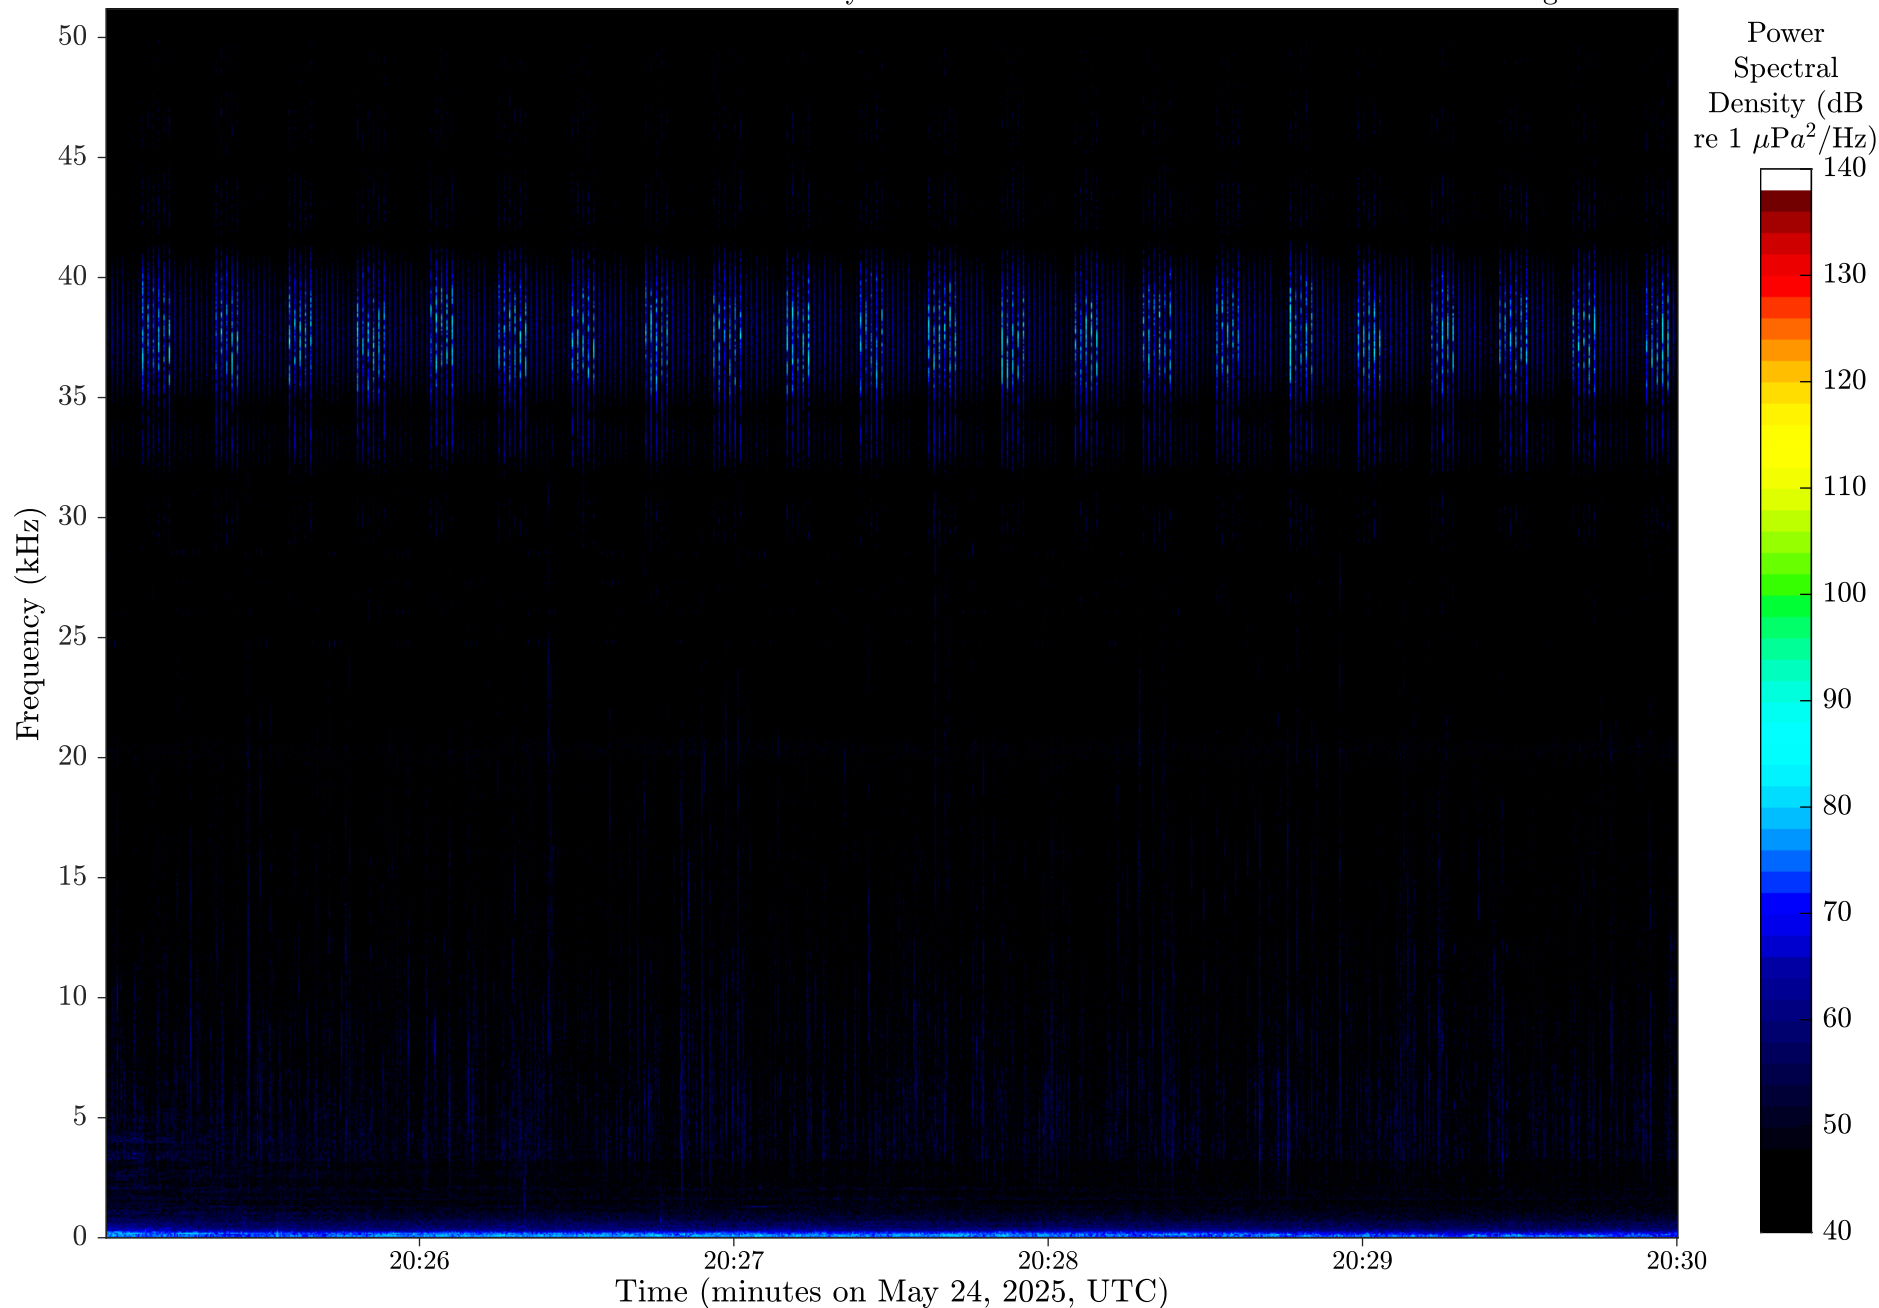


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:48:56 UTC

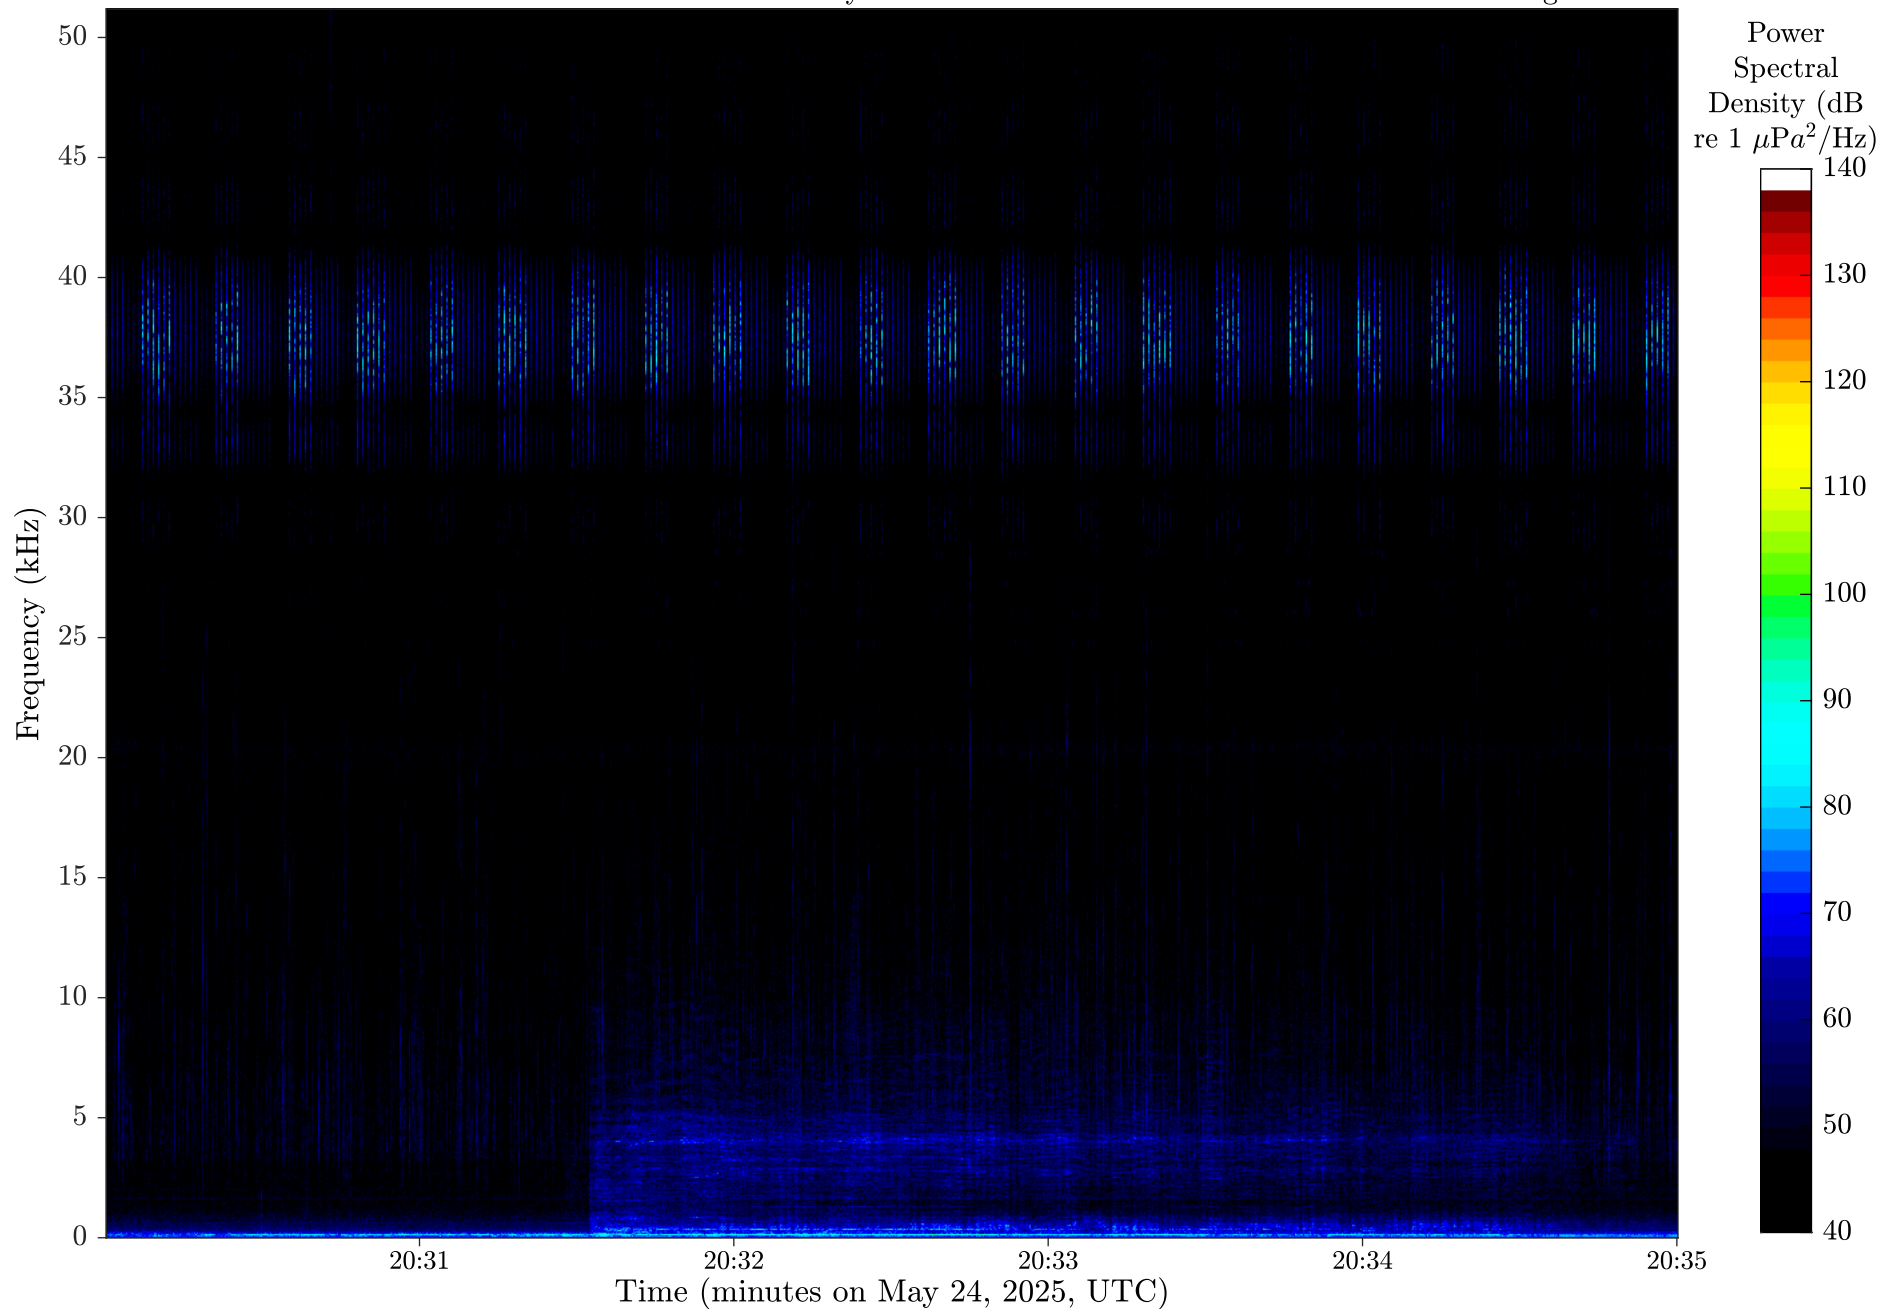


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:05 UTC

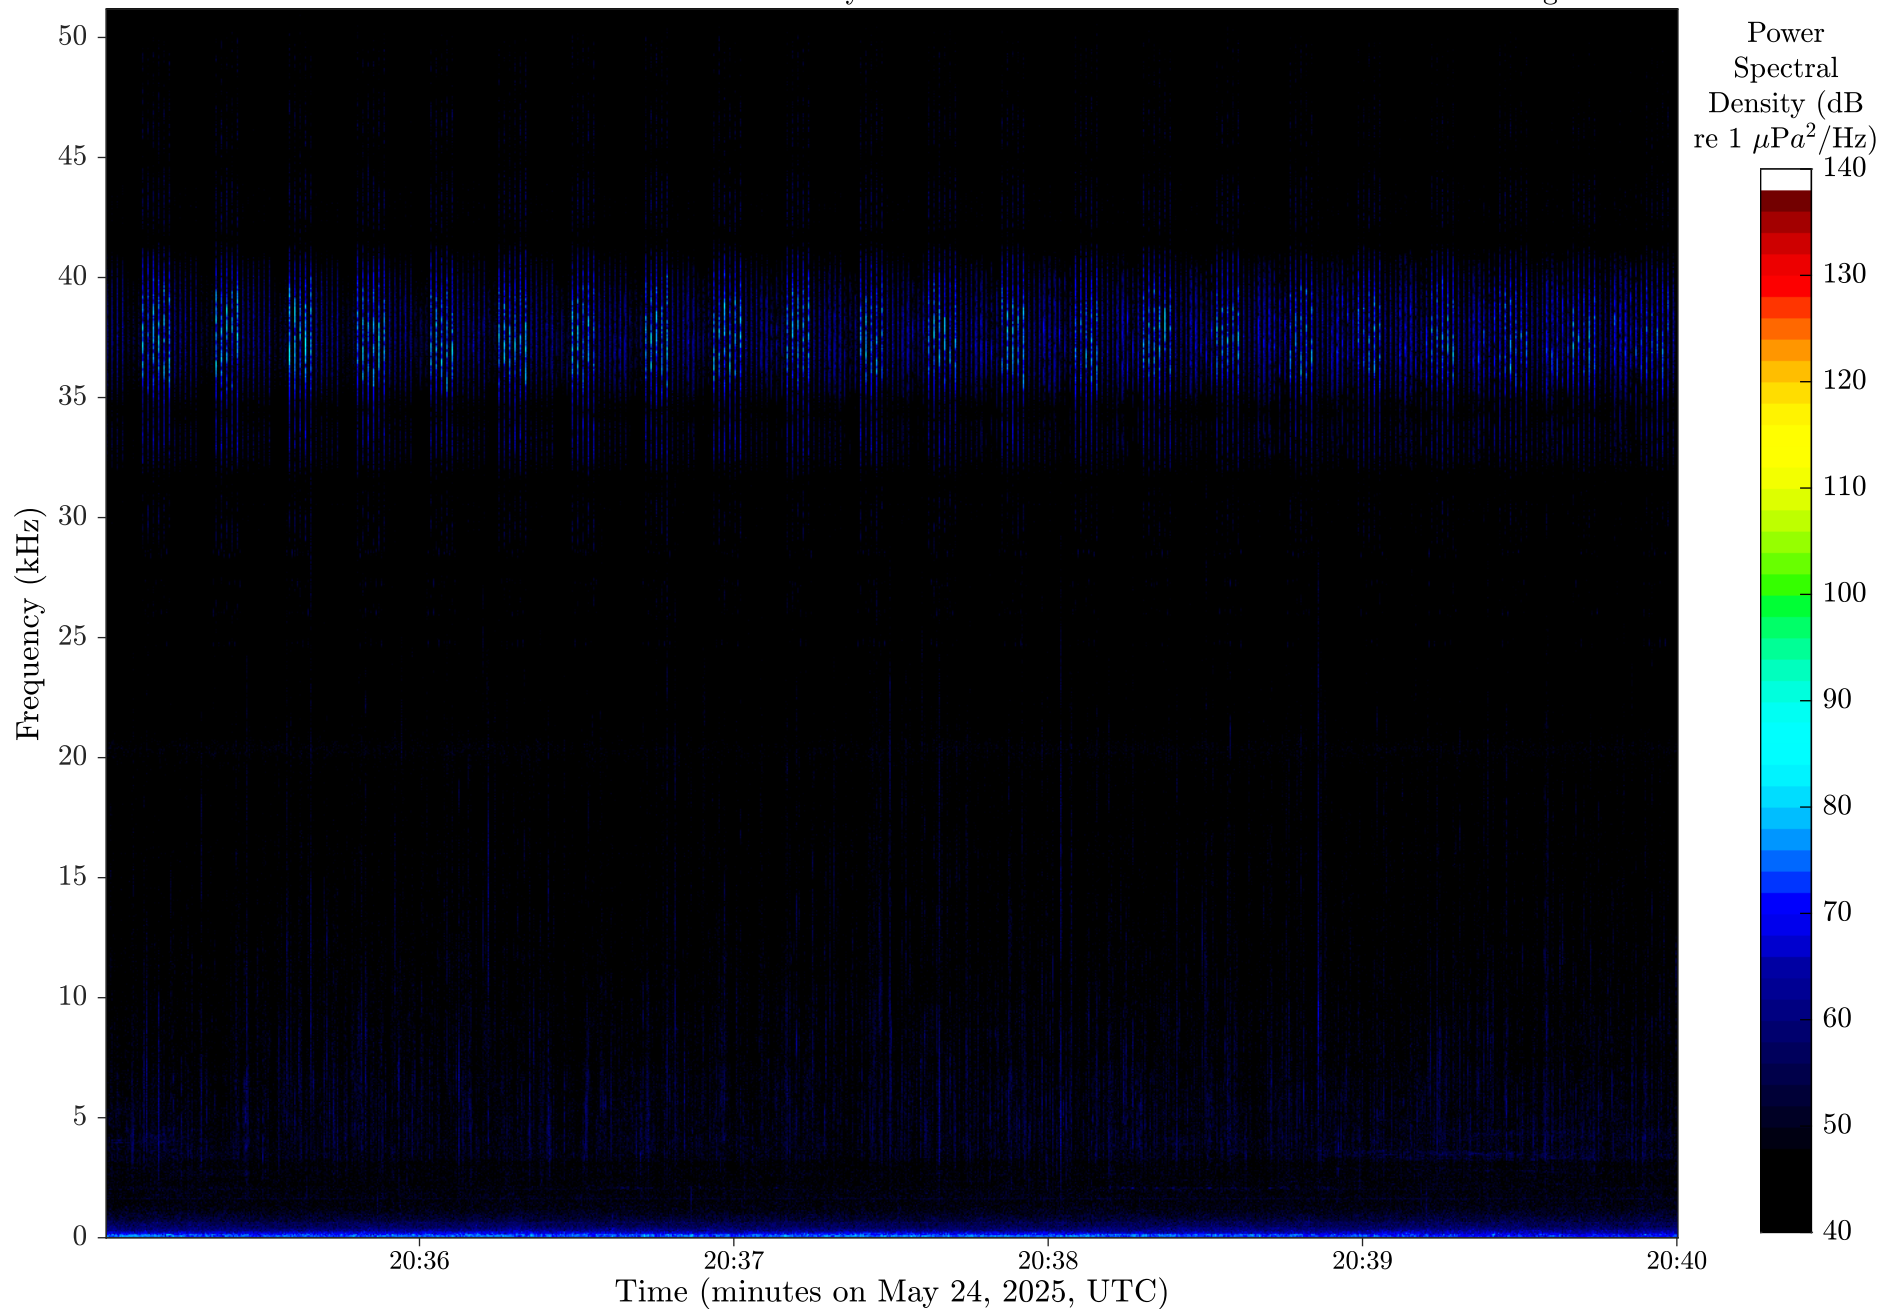


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:13 UTC

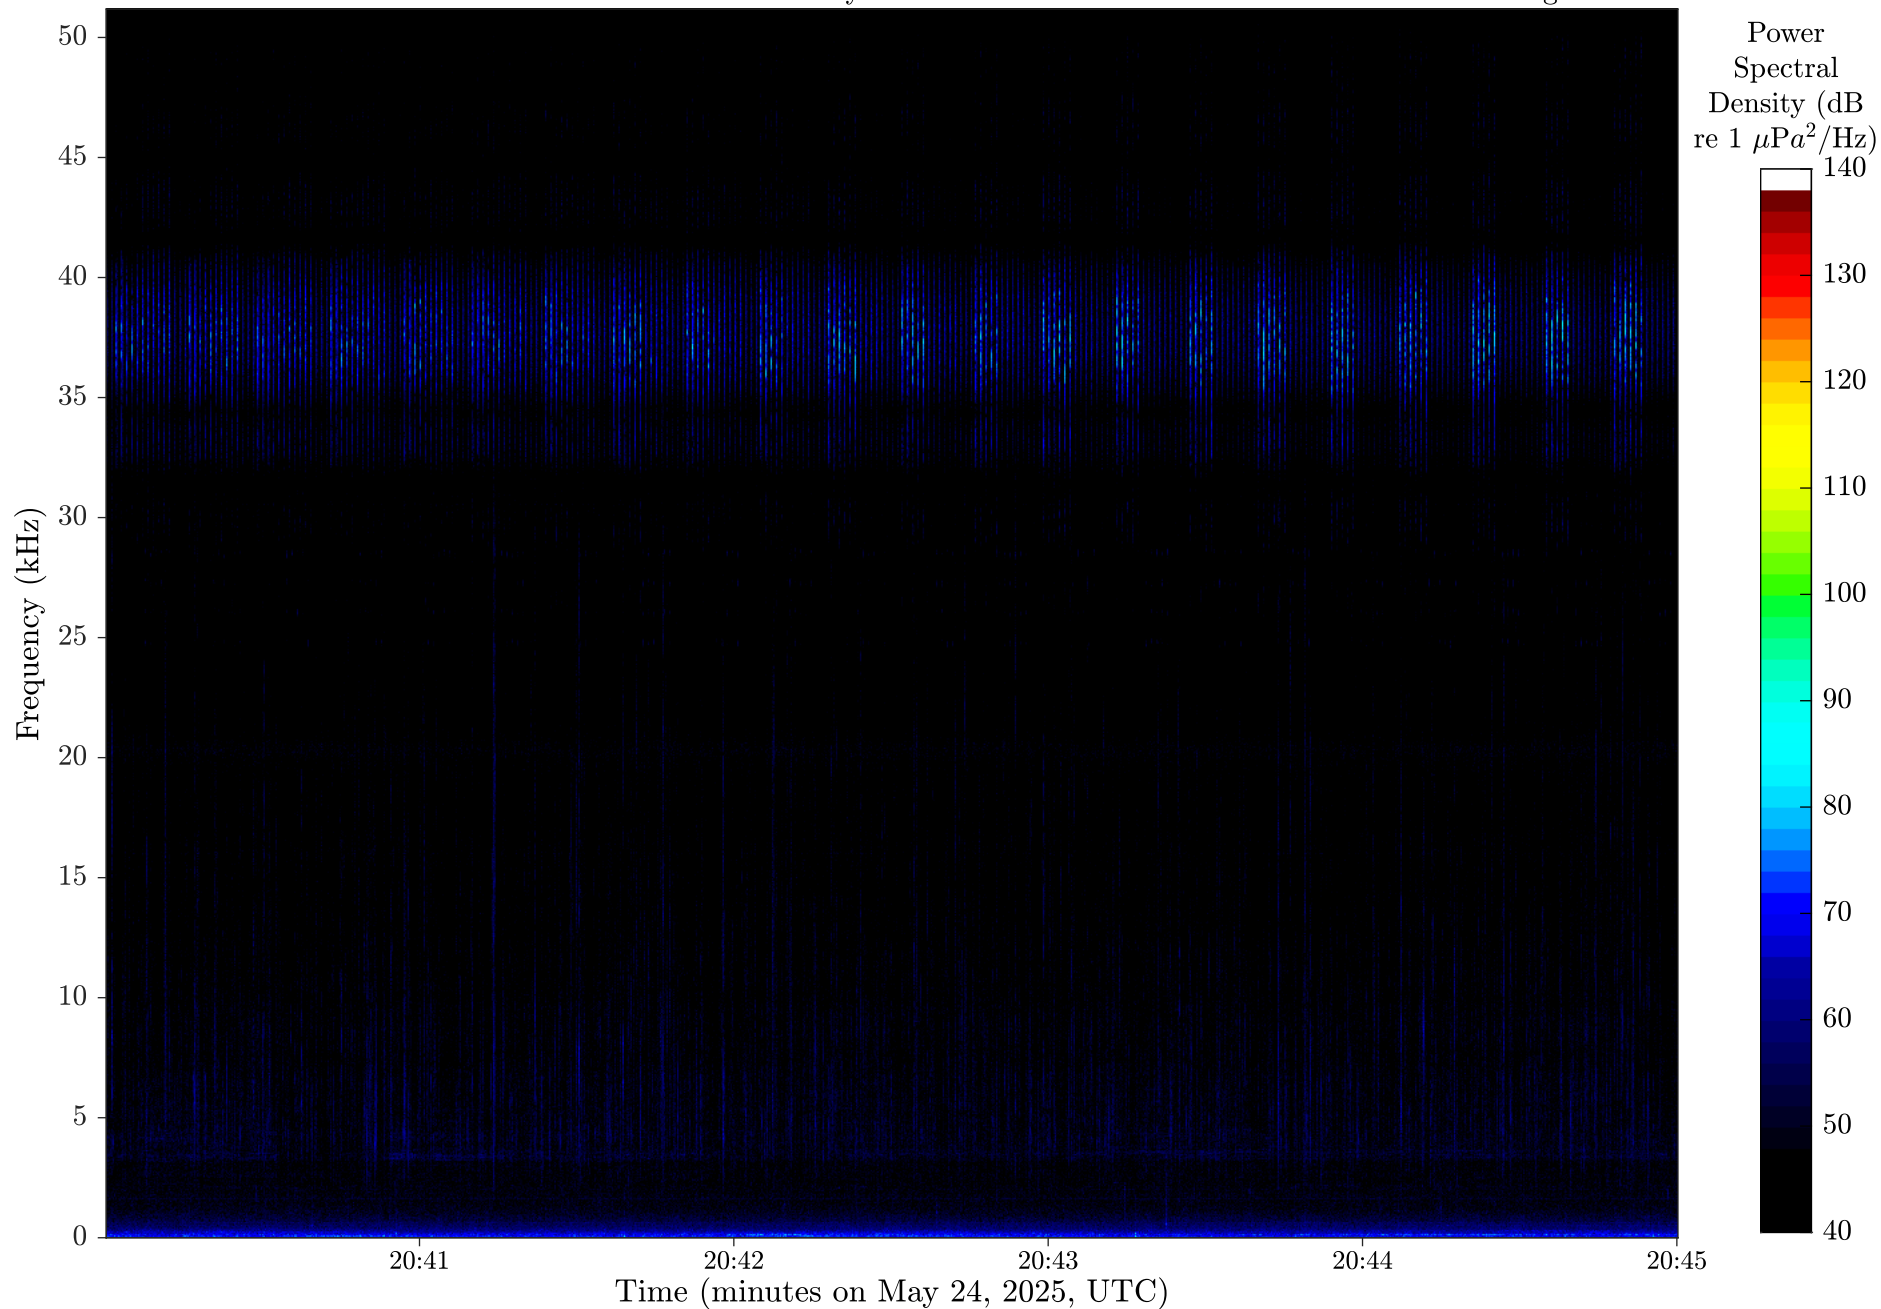


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:22 UTC

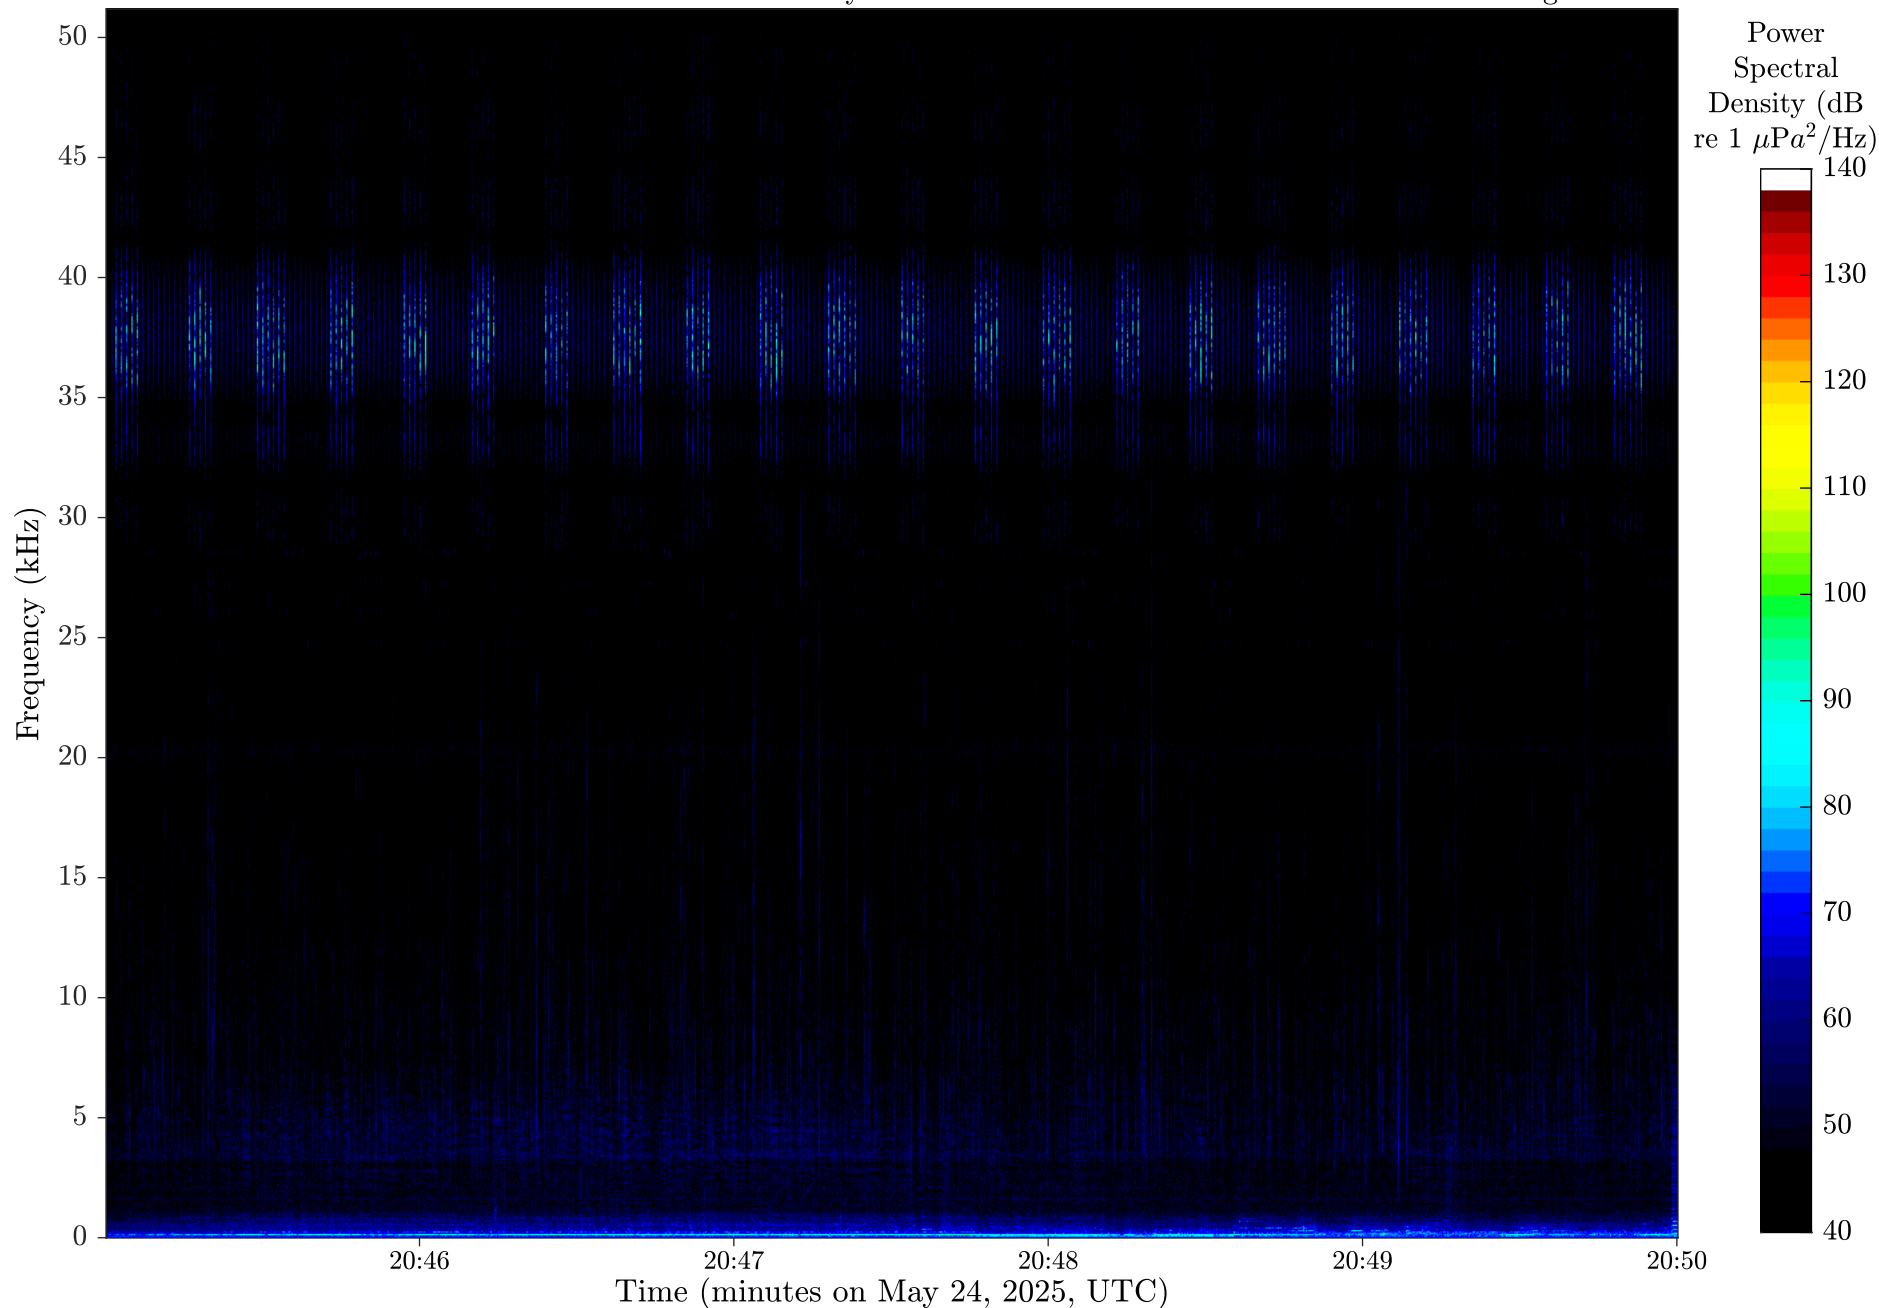


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:30 UTC

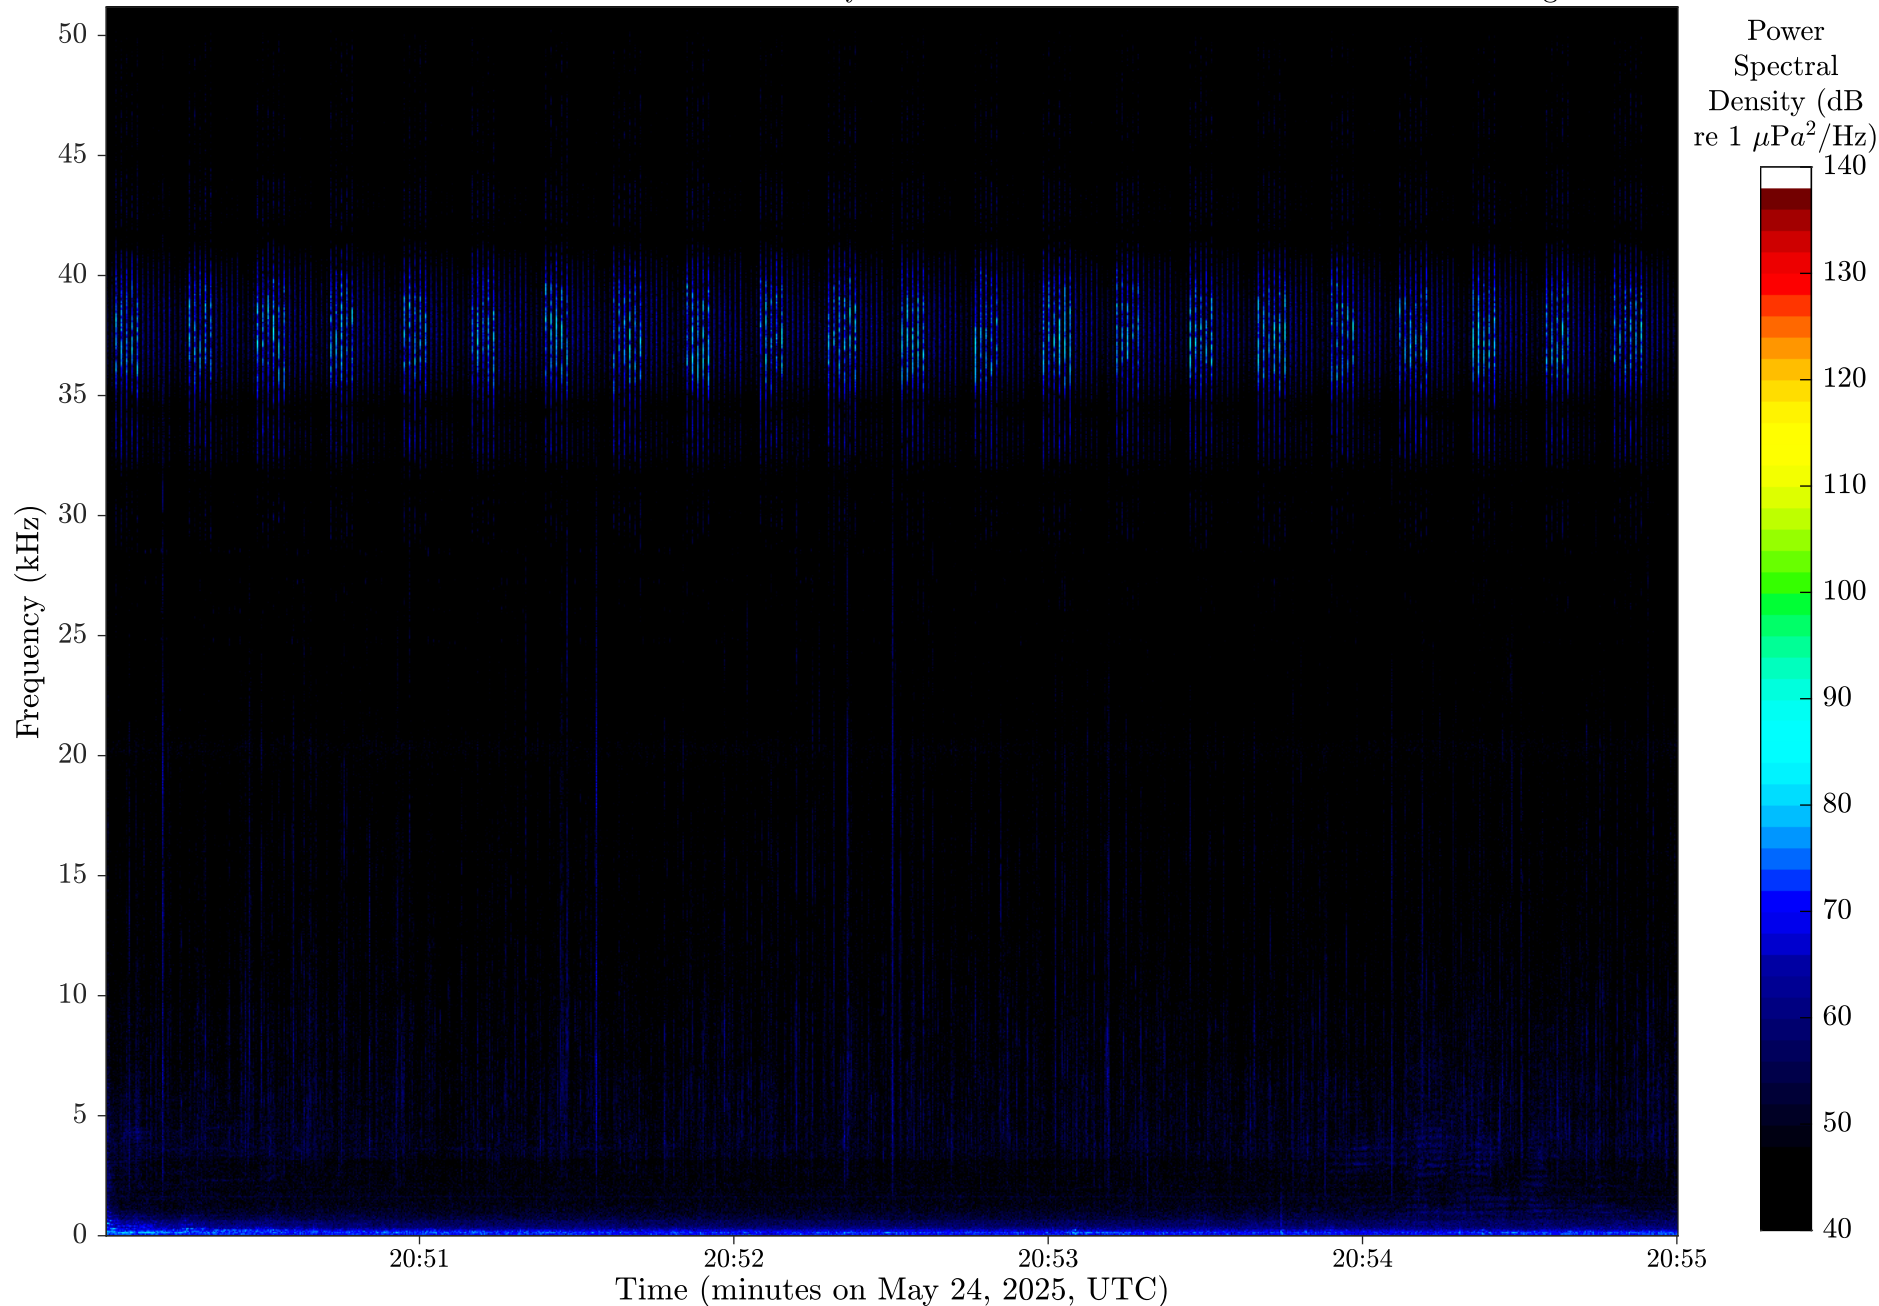


Comments: 33.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:38 UTC

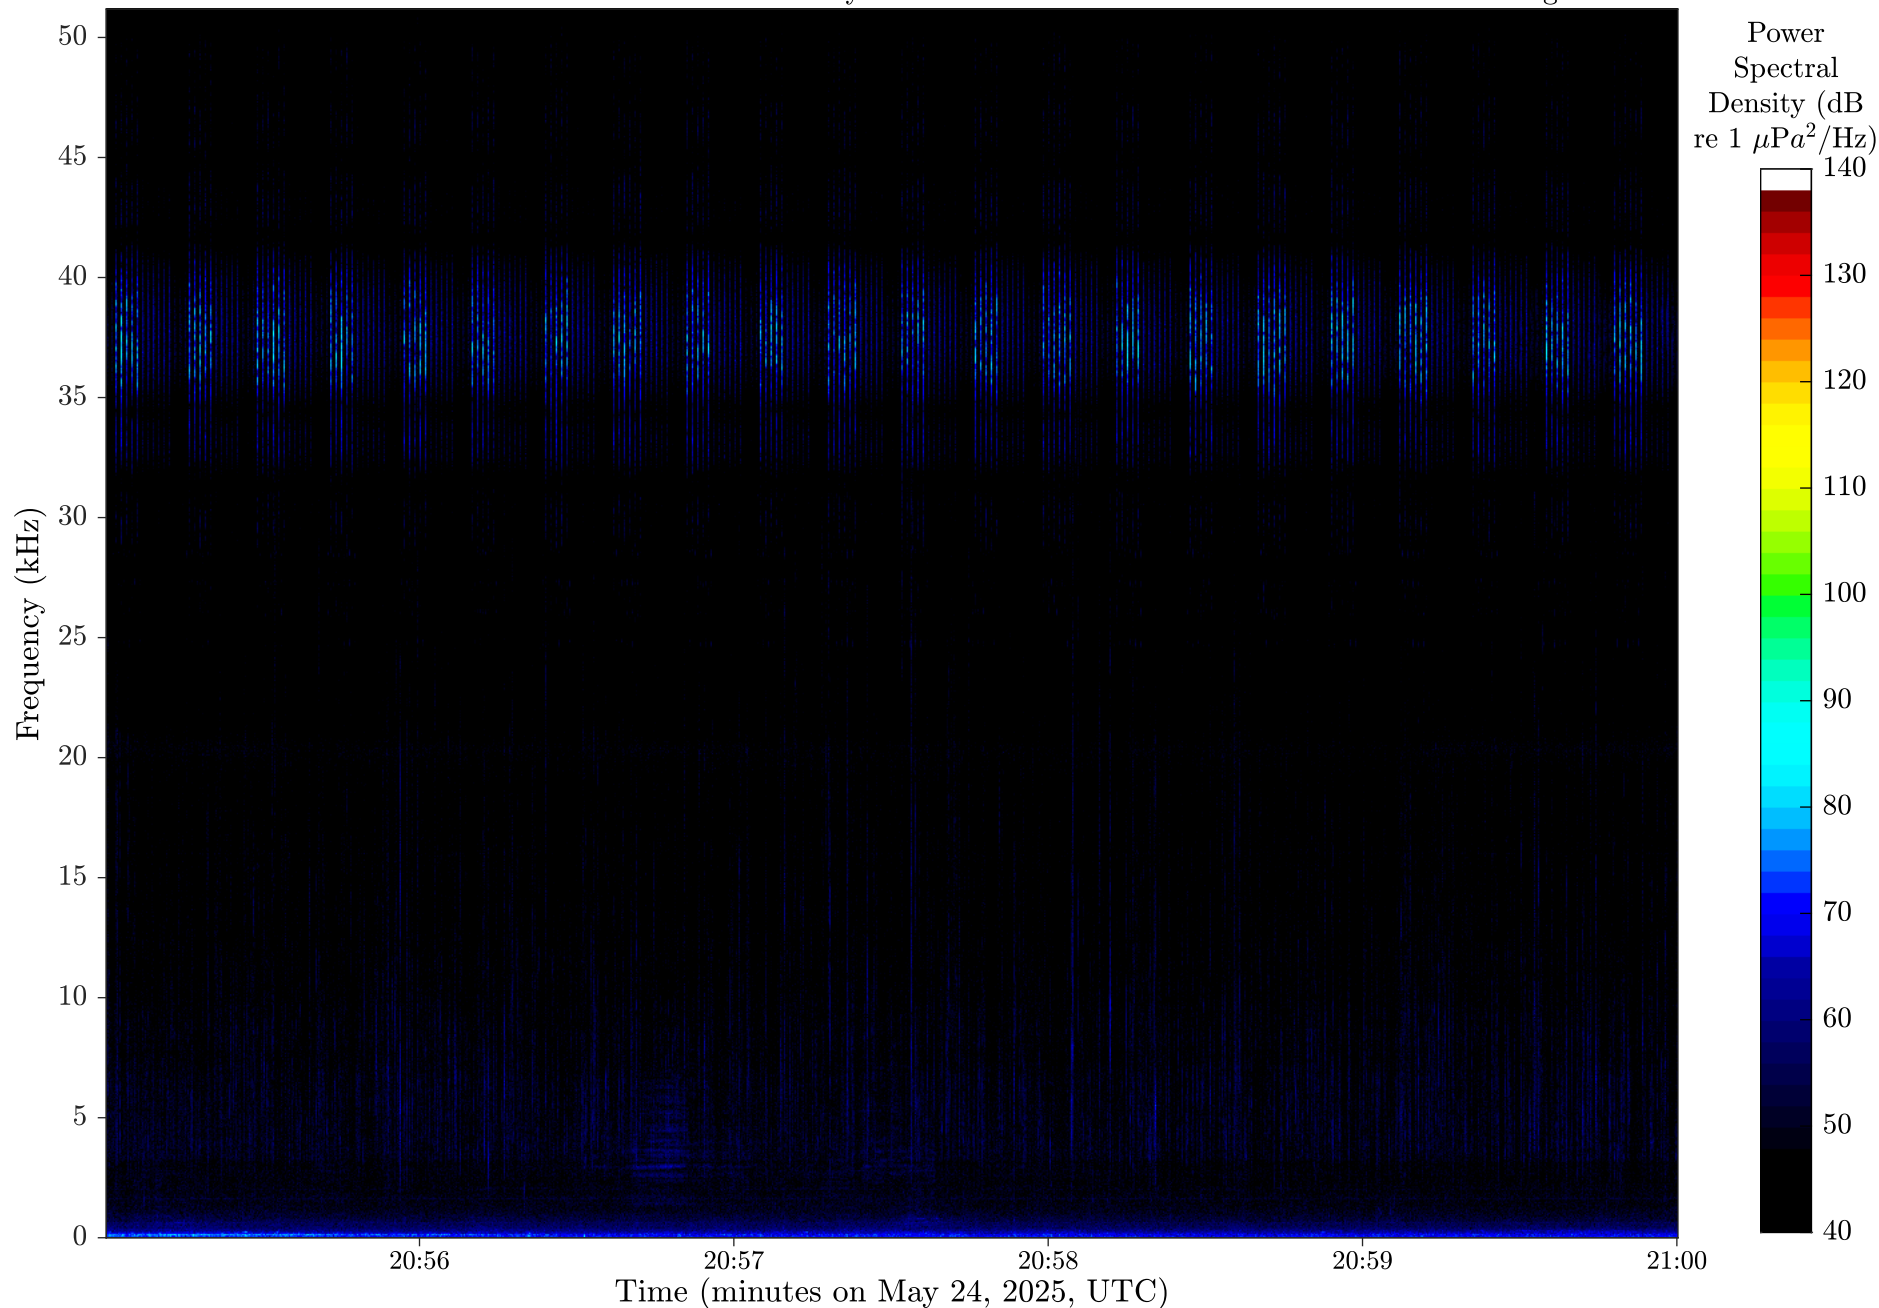


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:46 UTC

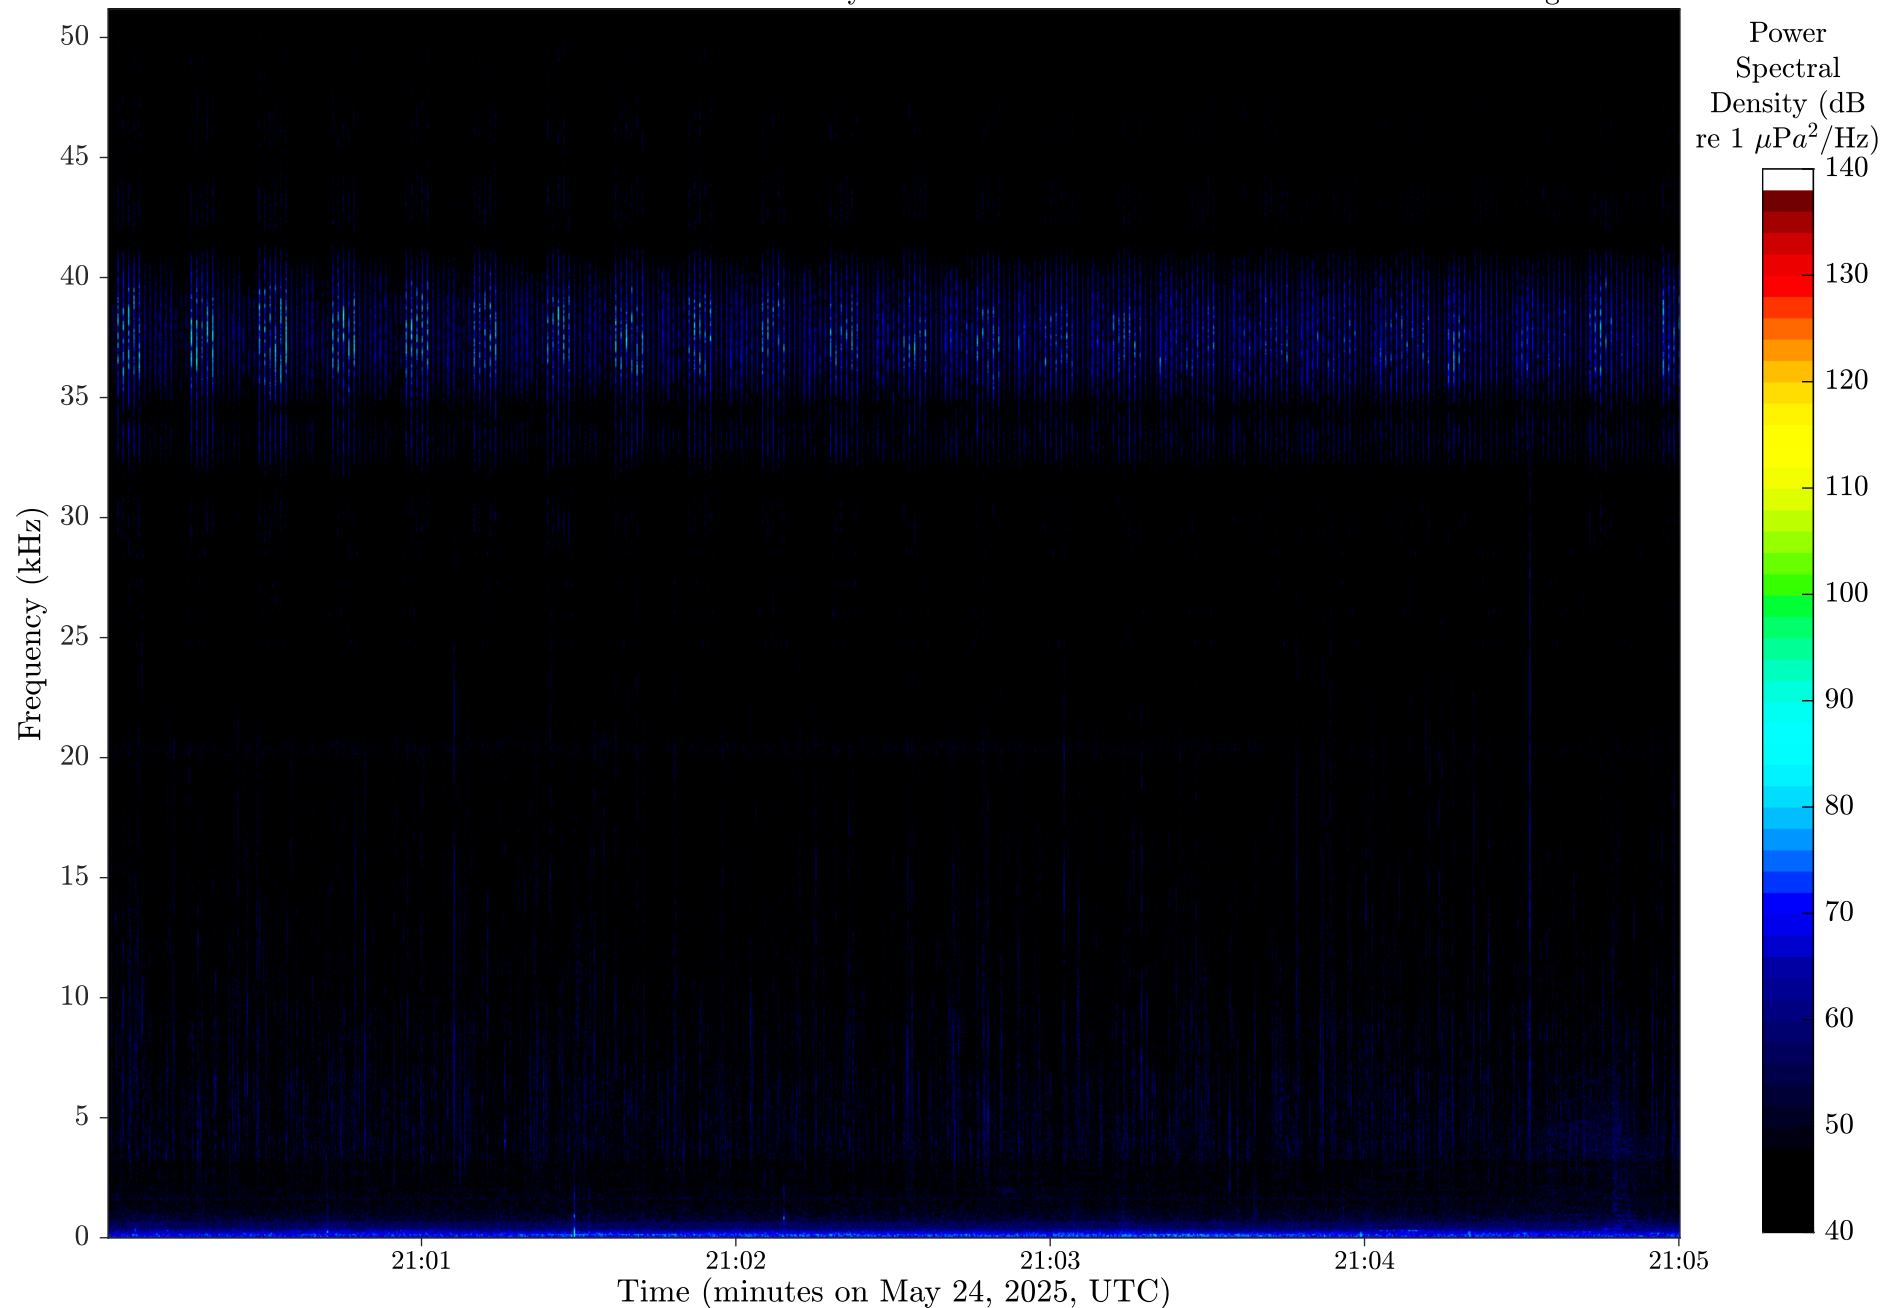


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:54 UTC

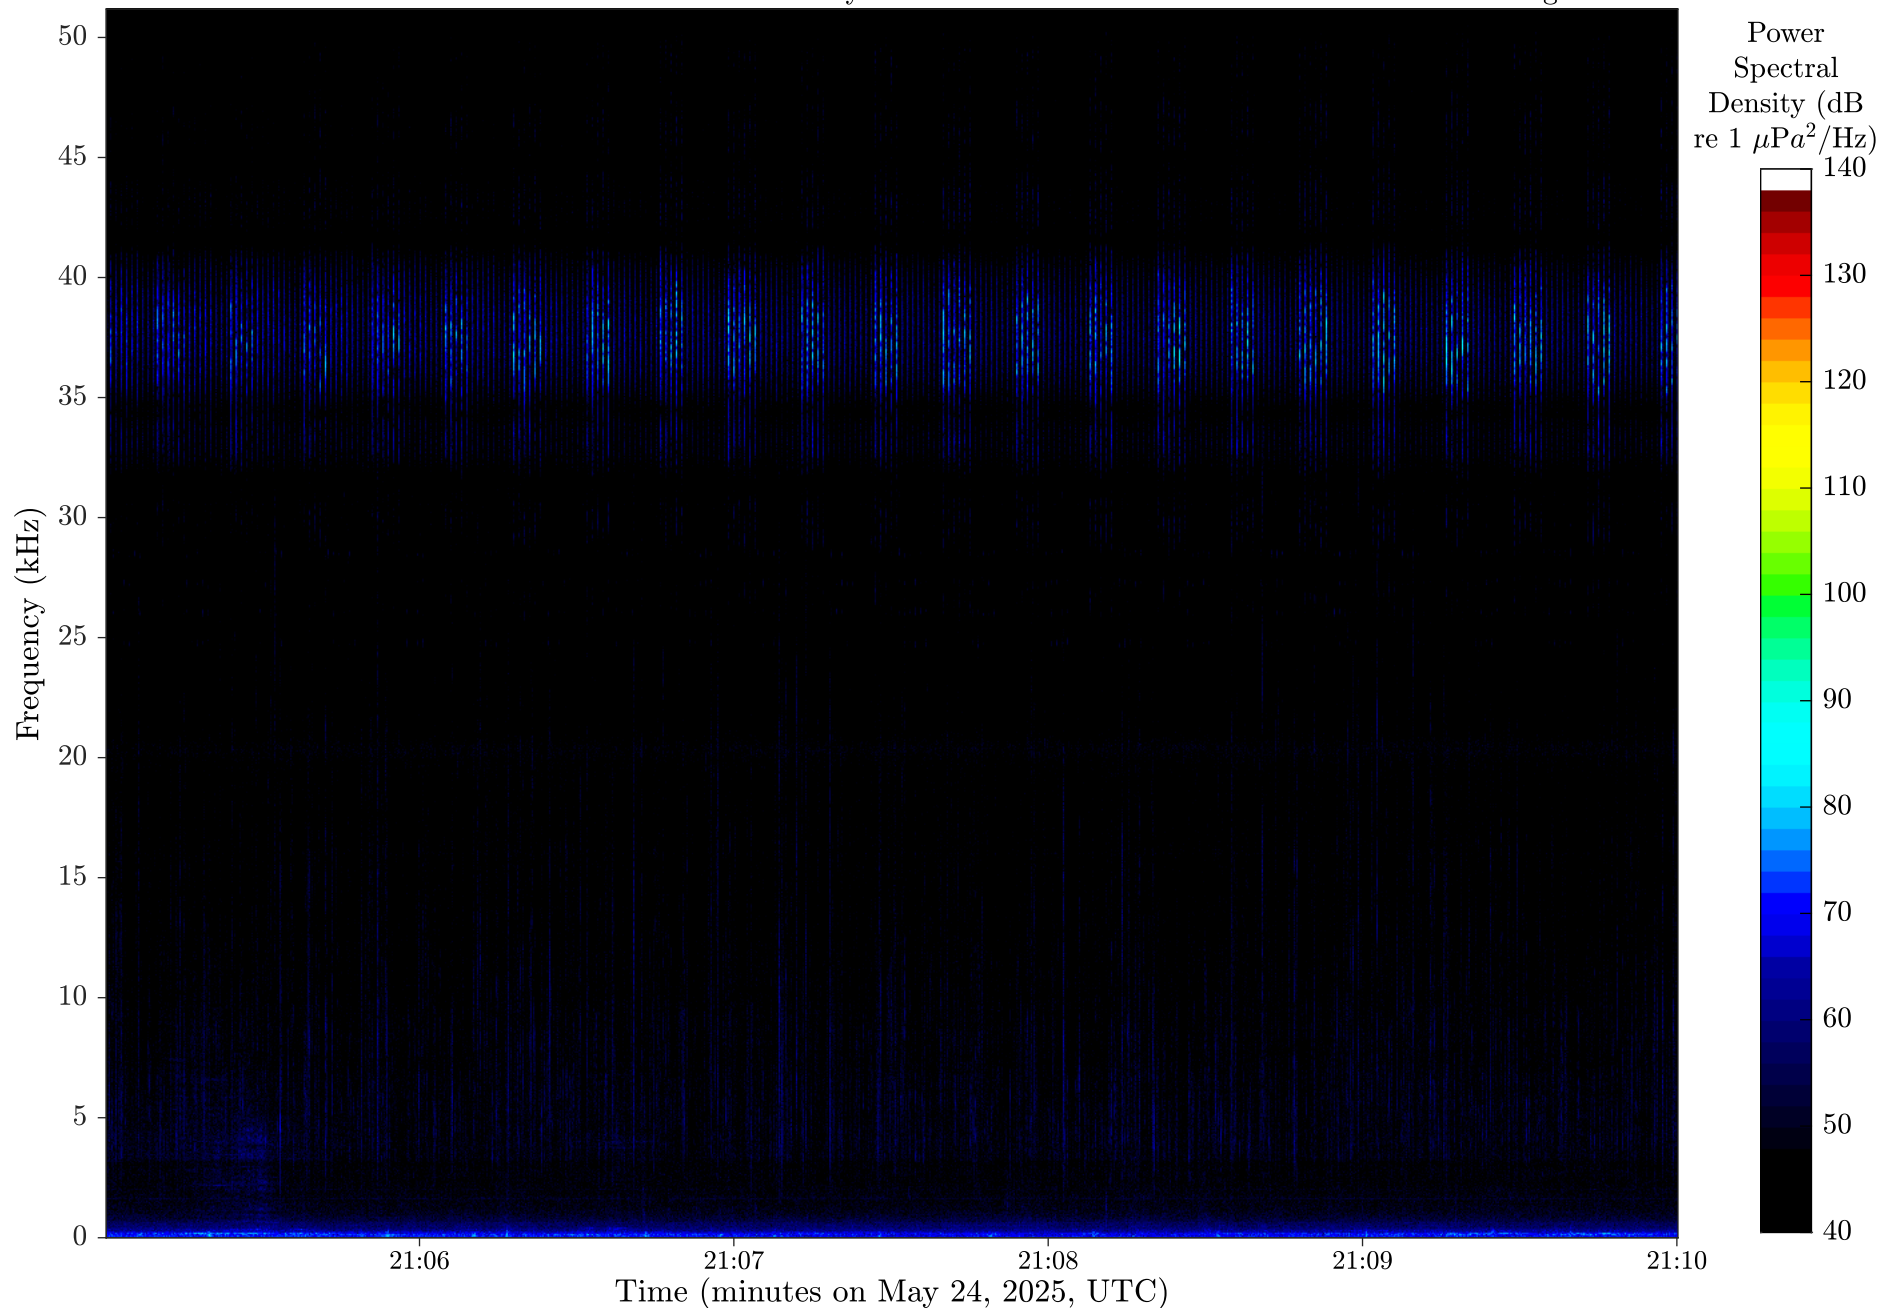


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:50:02 UTC

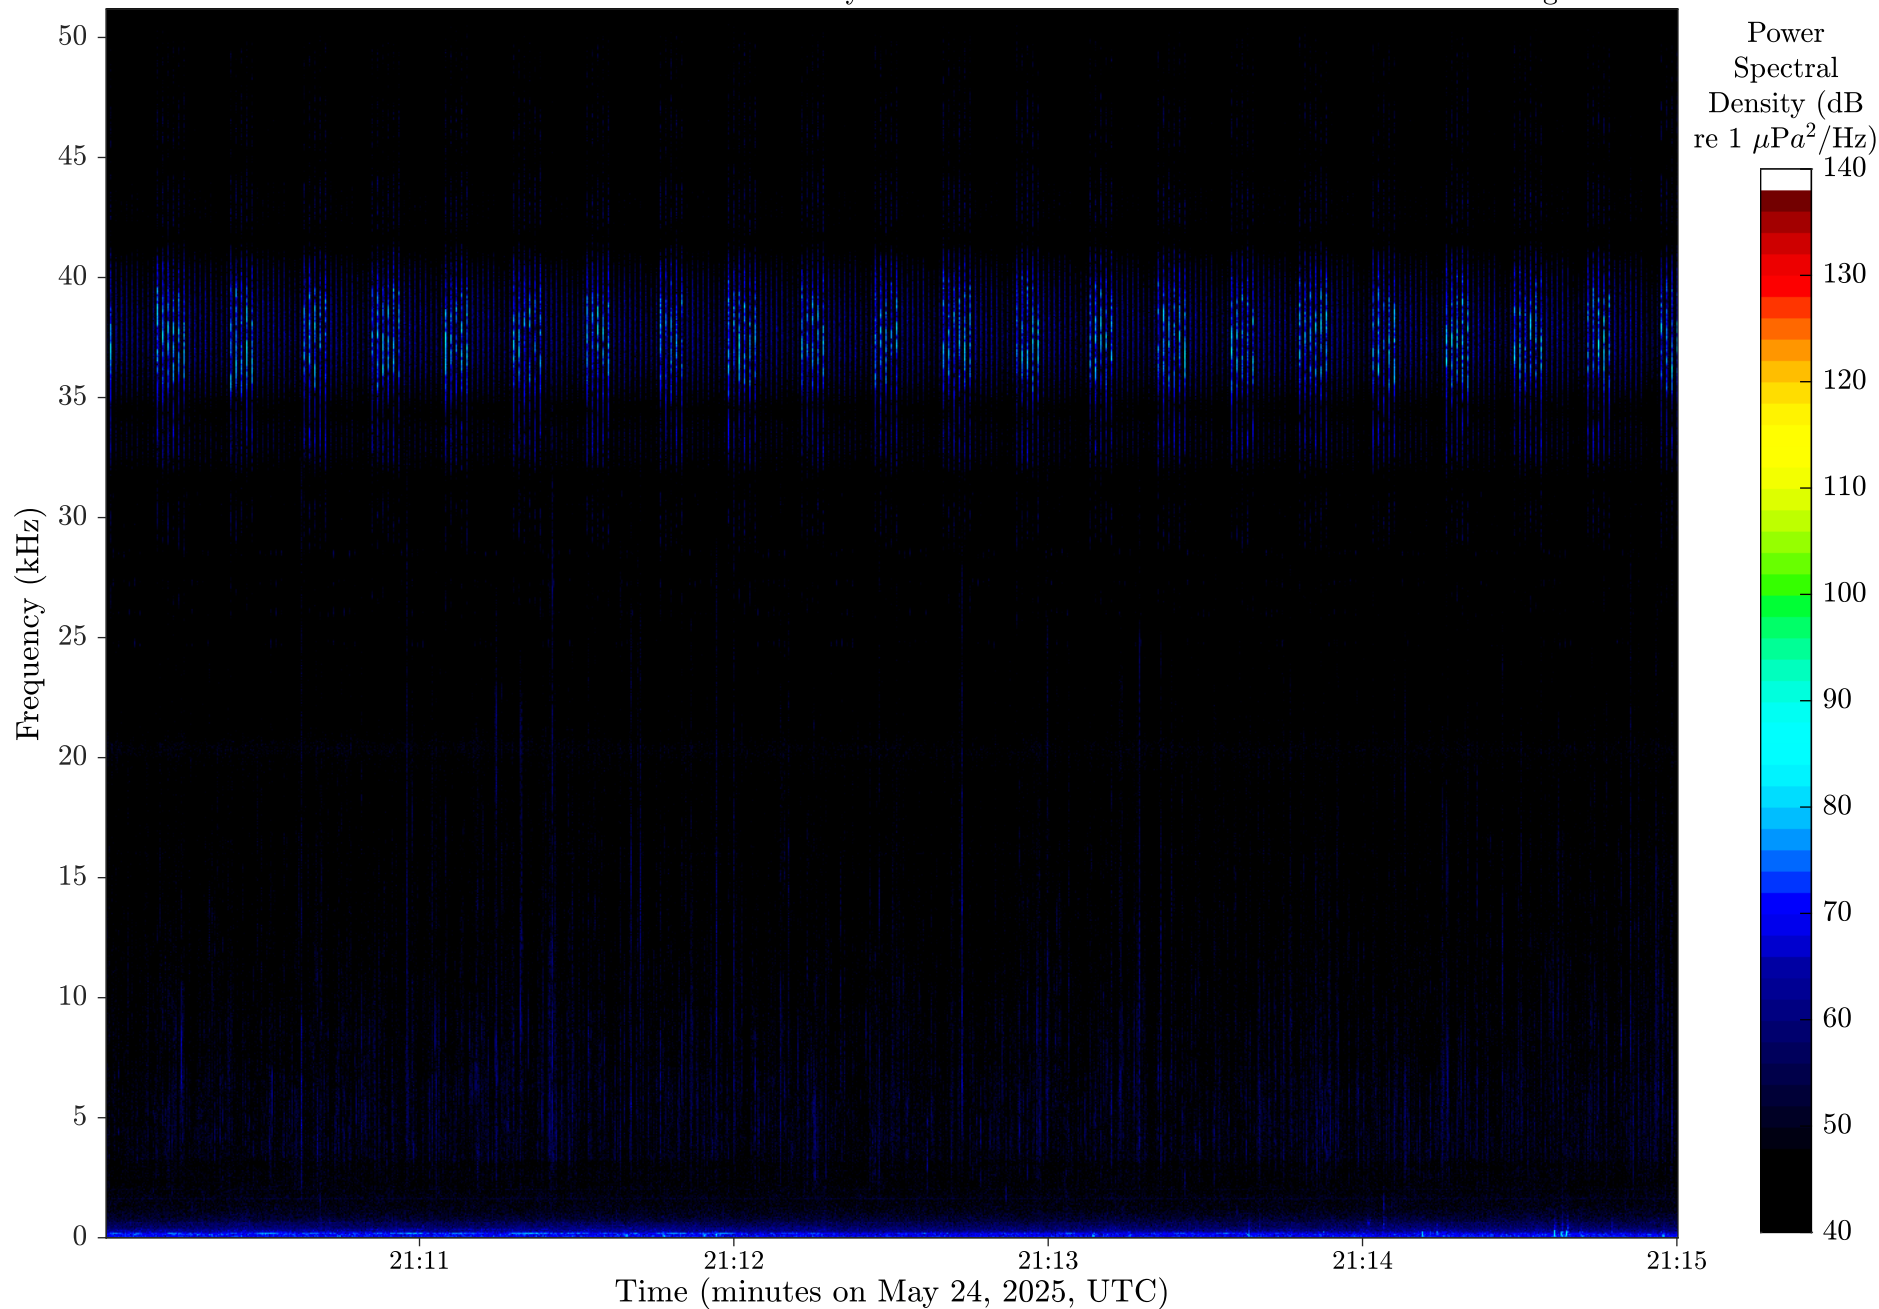


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:50:11 UTC

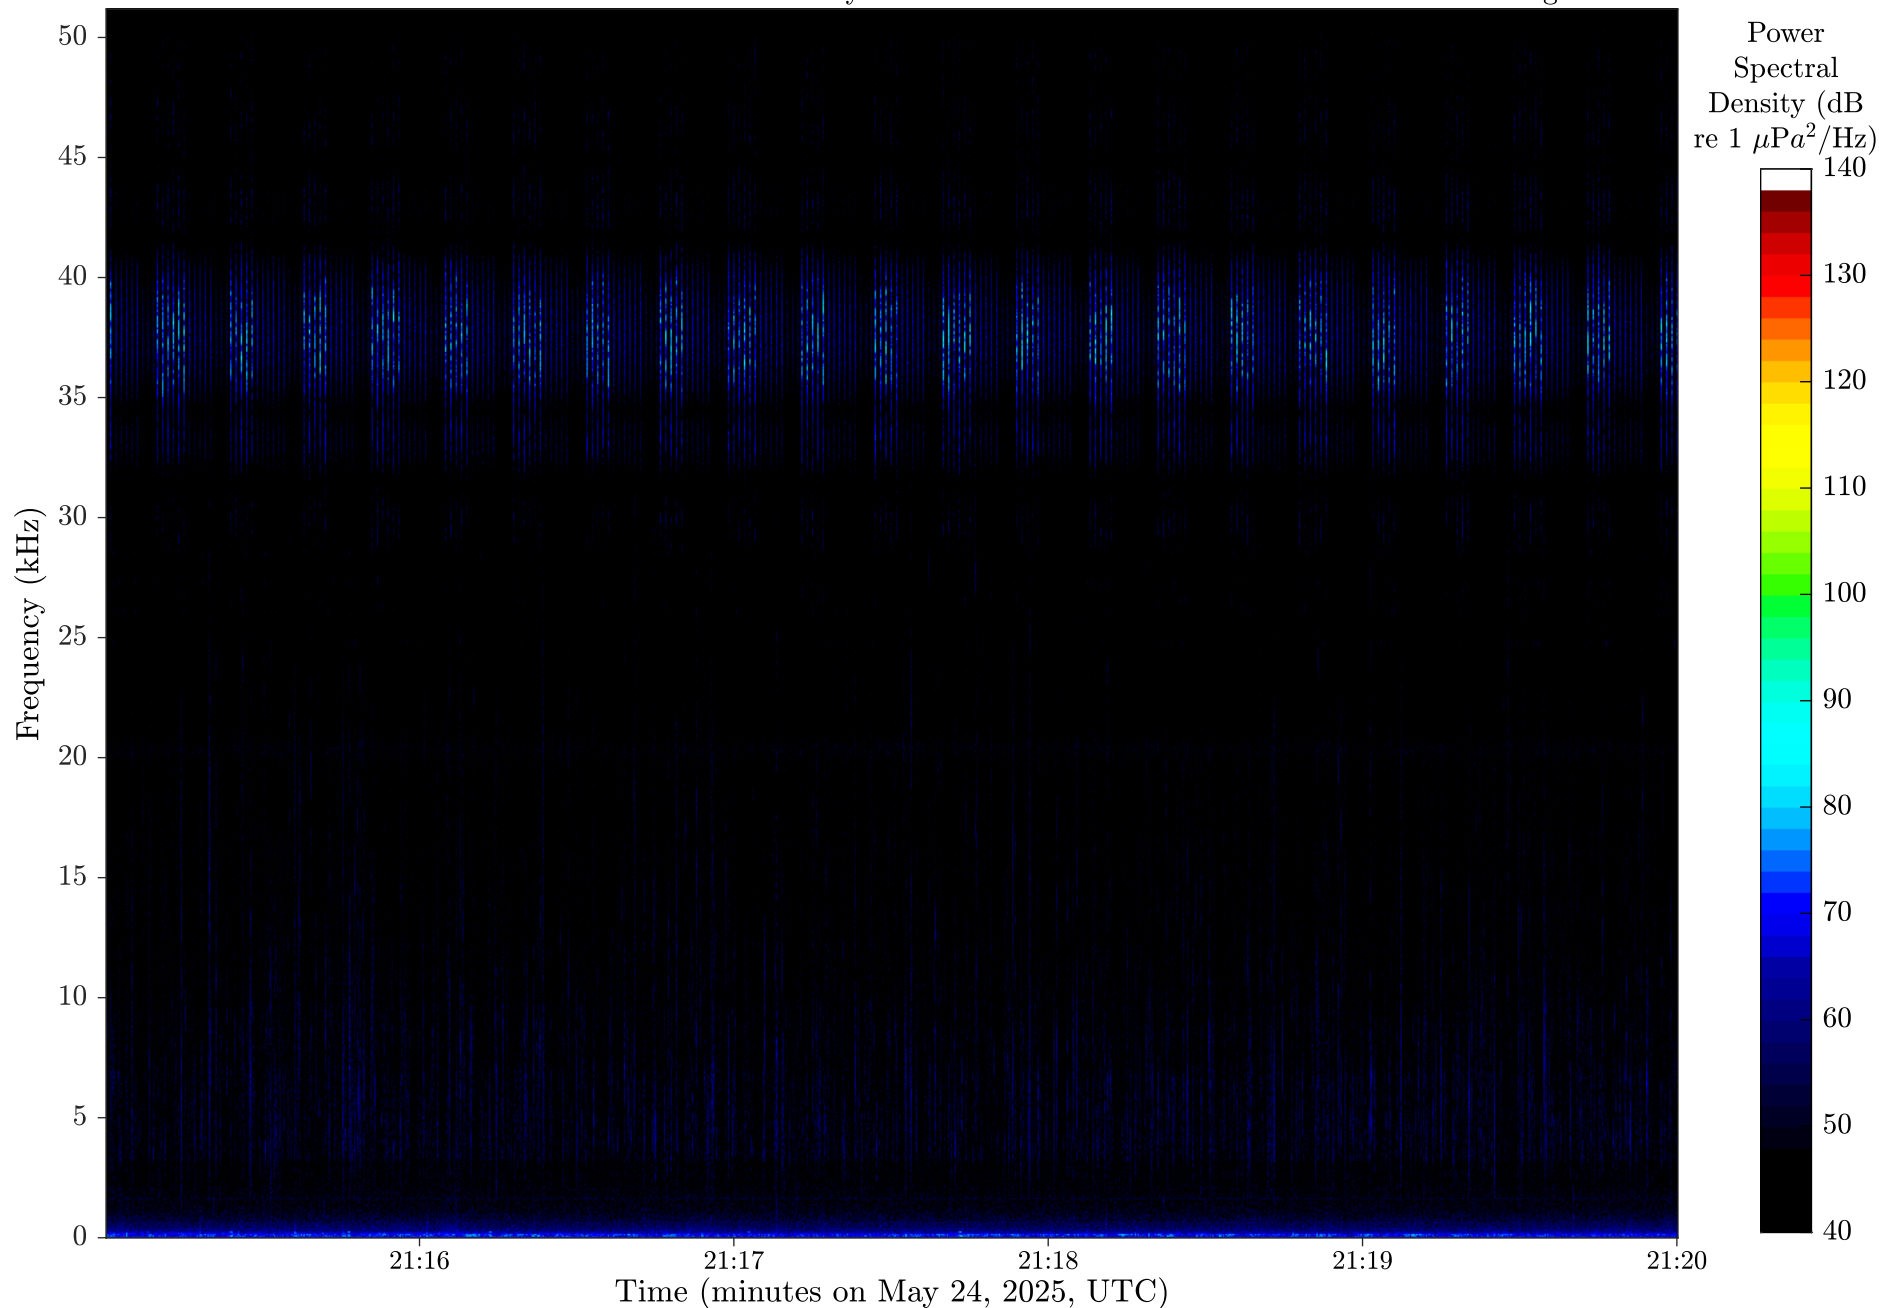


Comments: 34.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:50:20 UTC

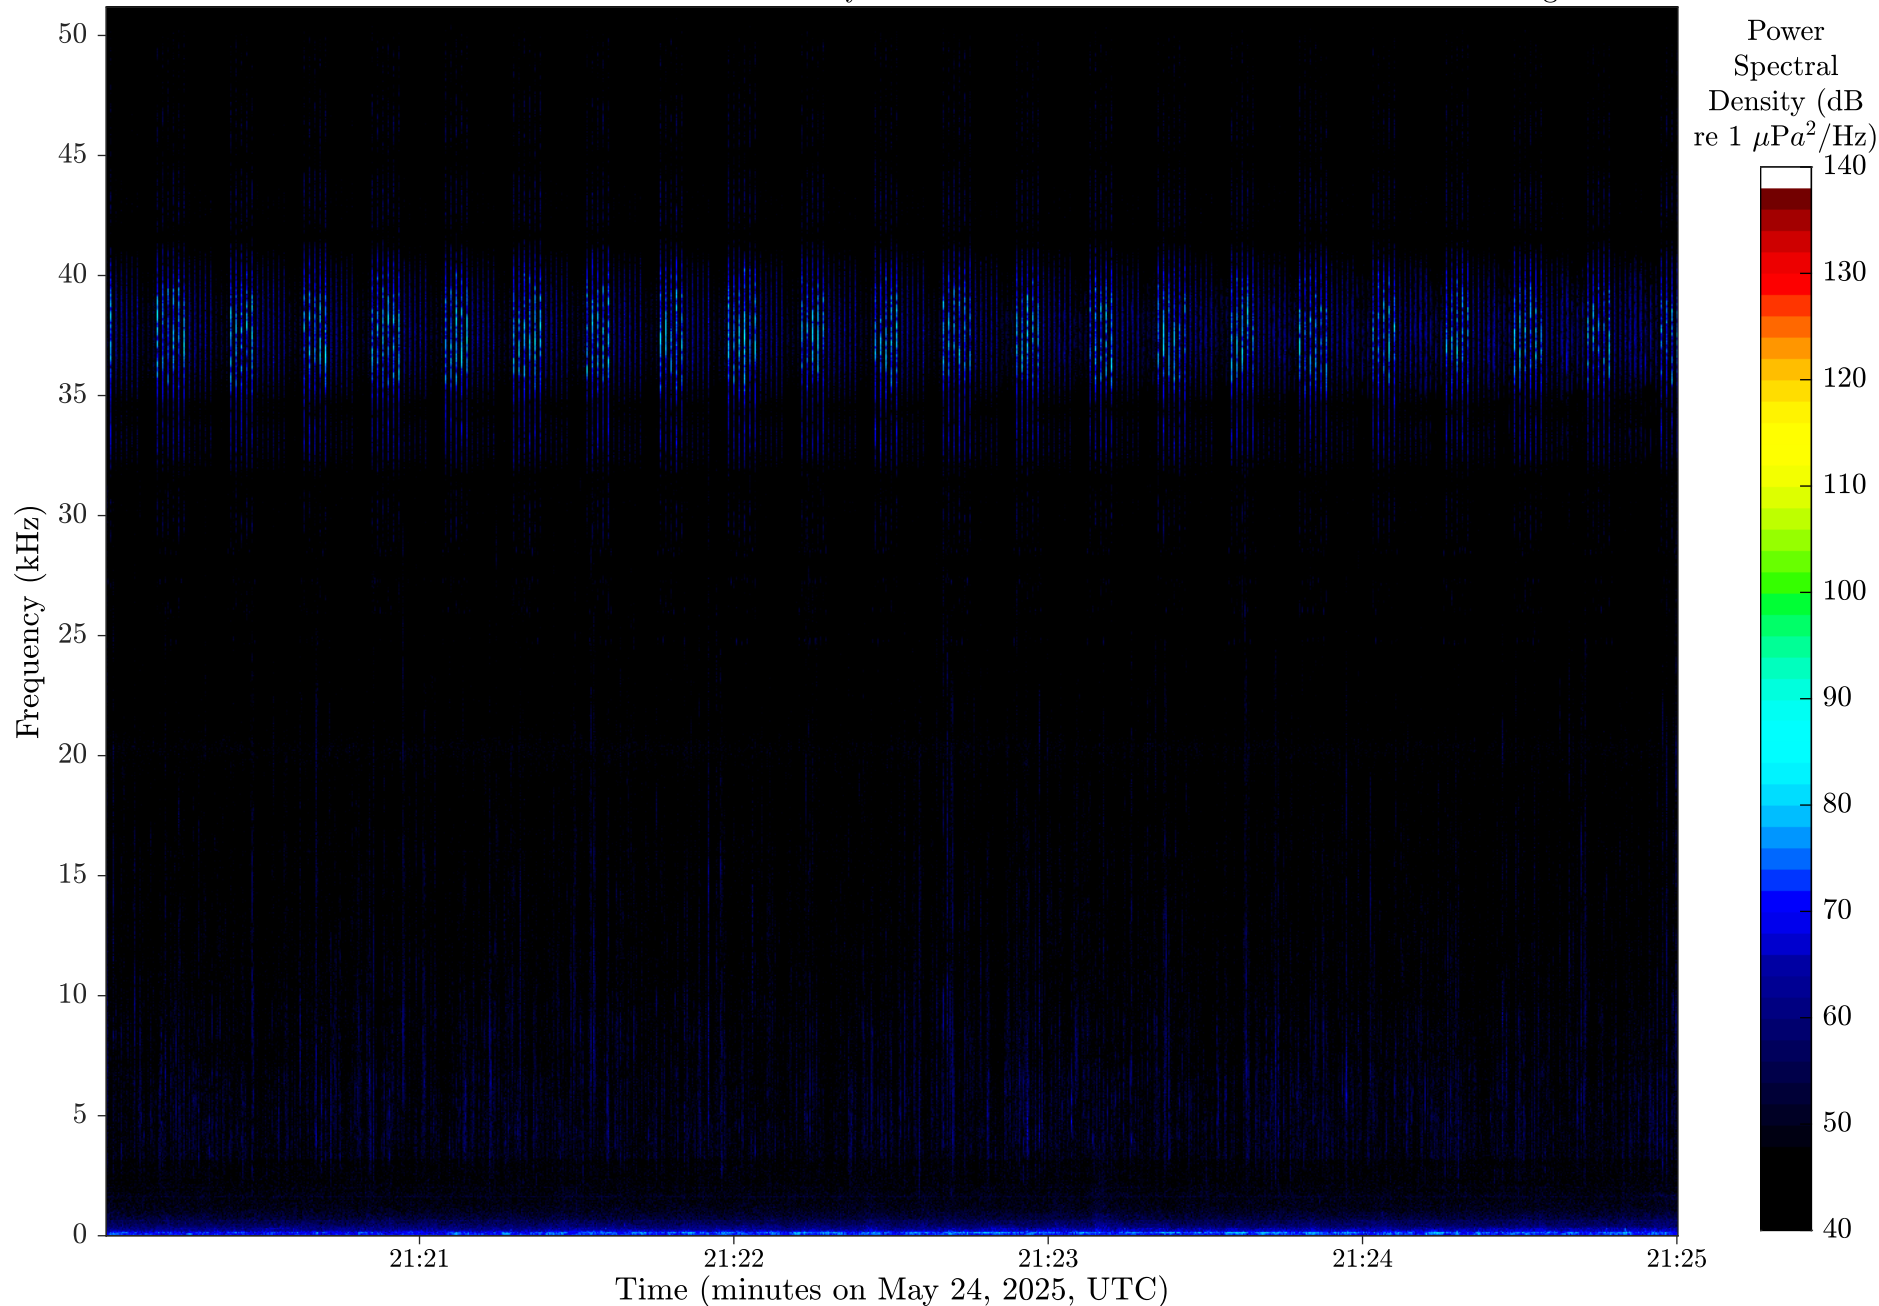


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:50:29 UTC

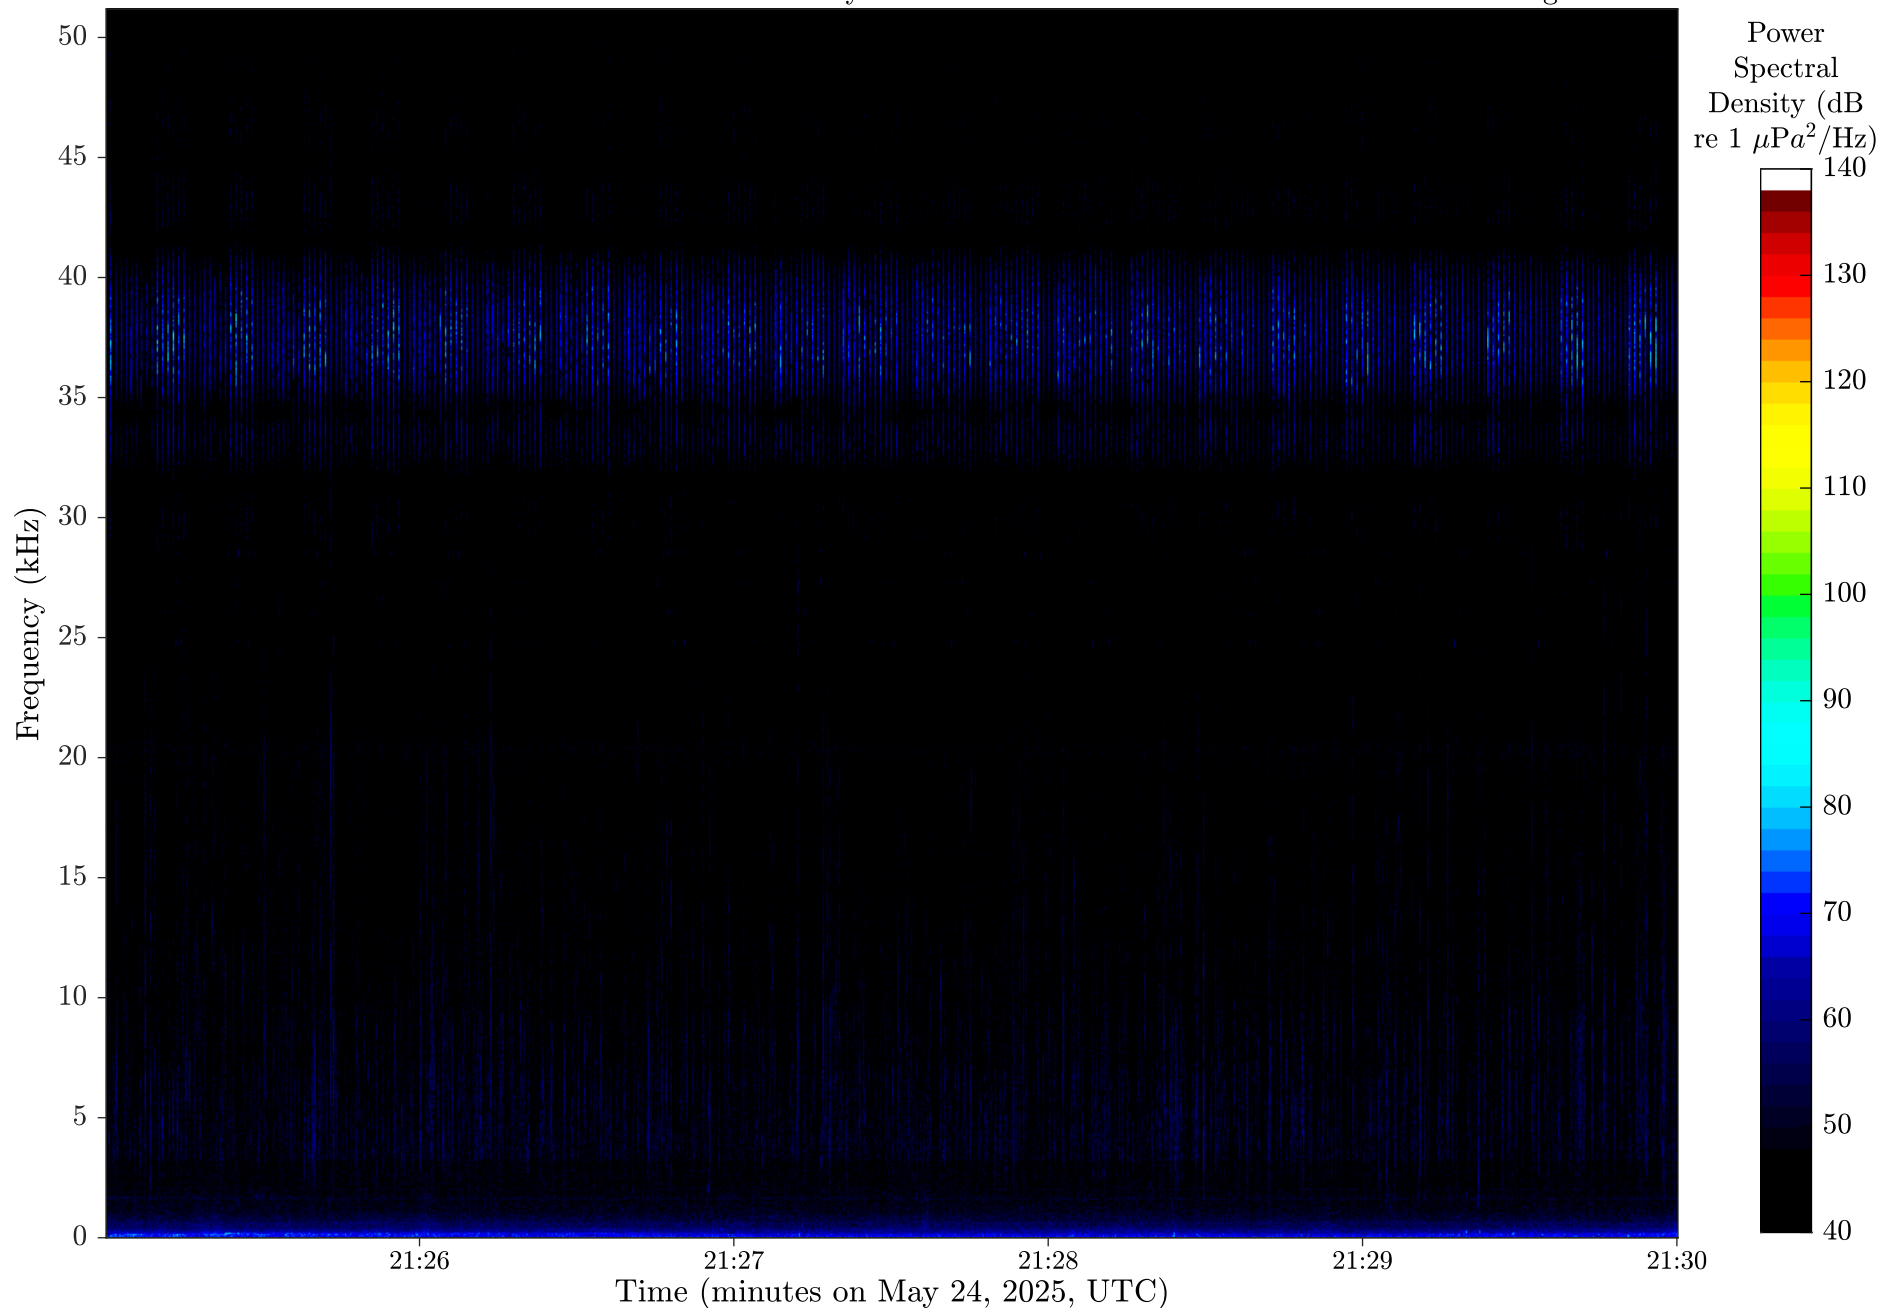


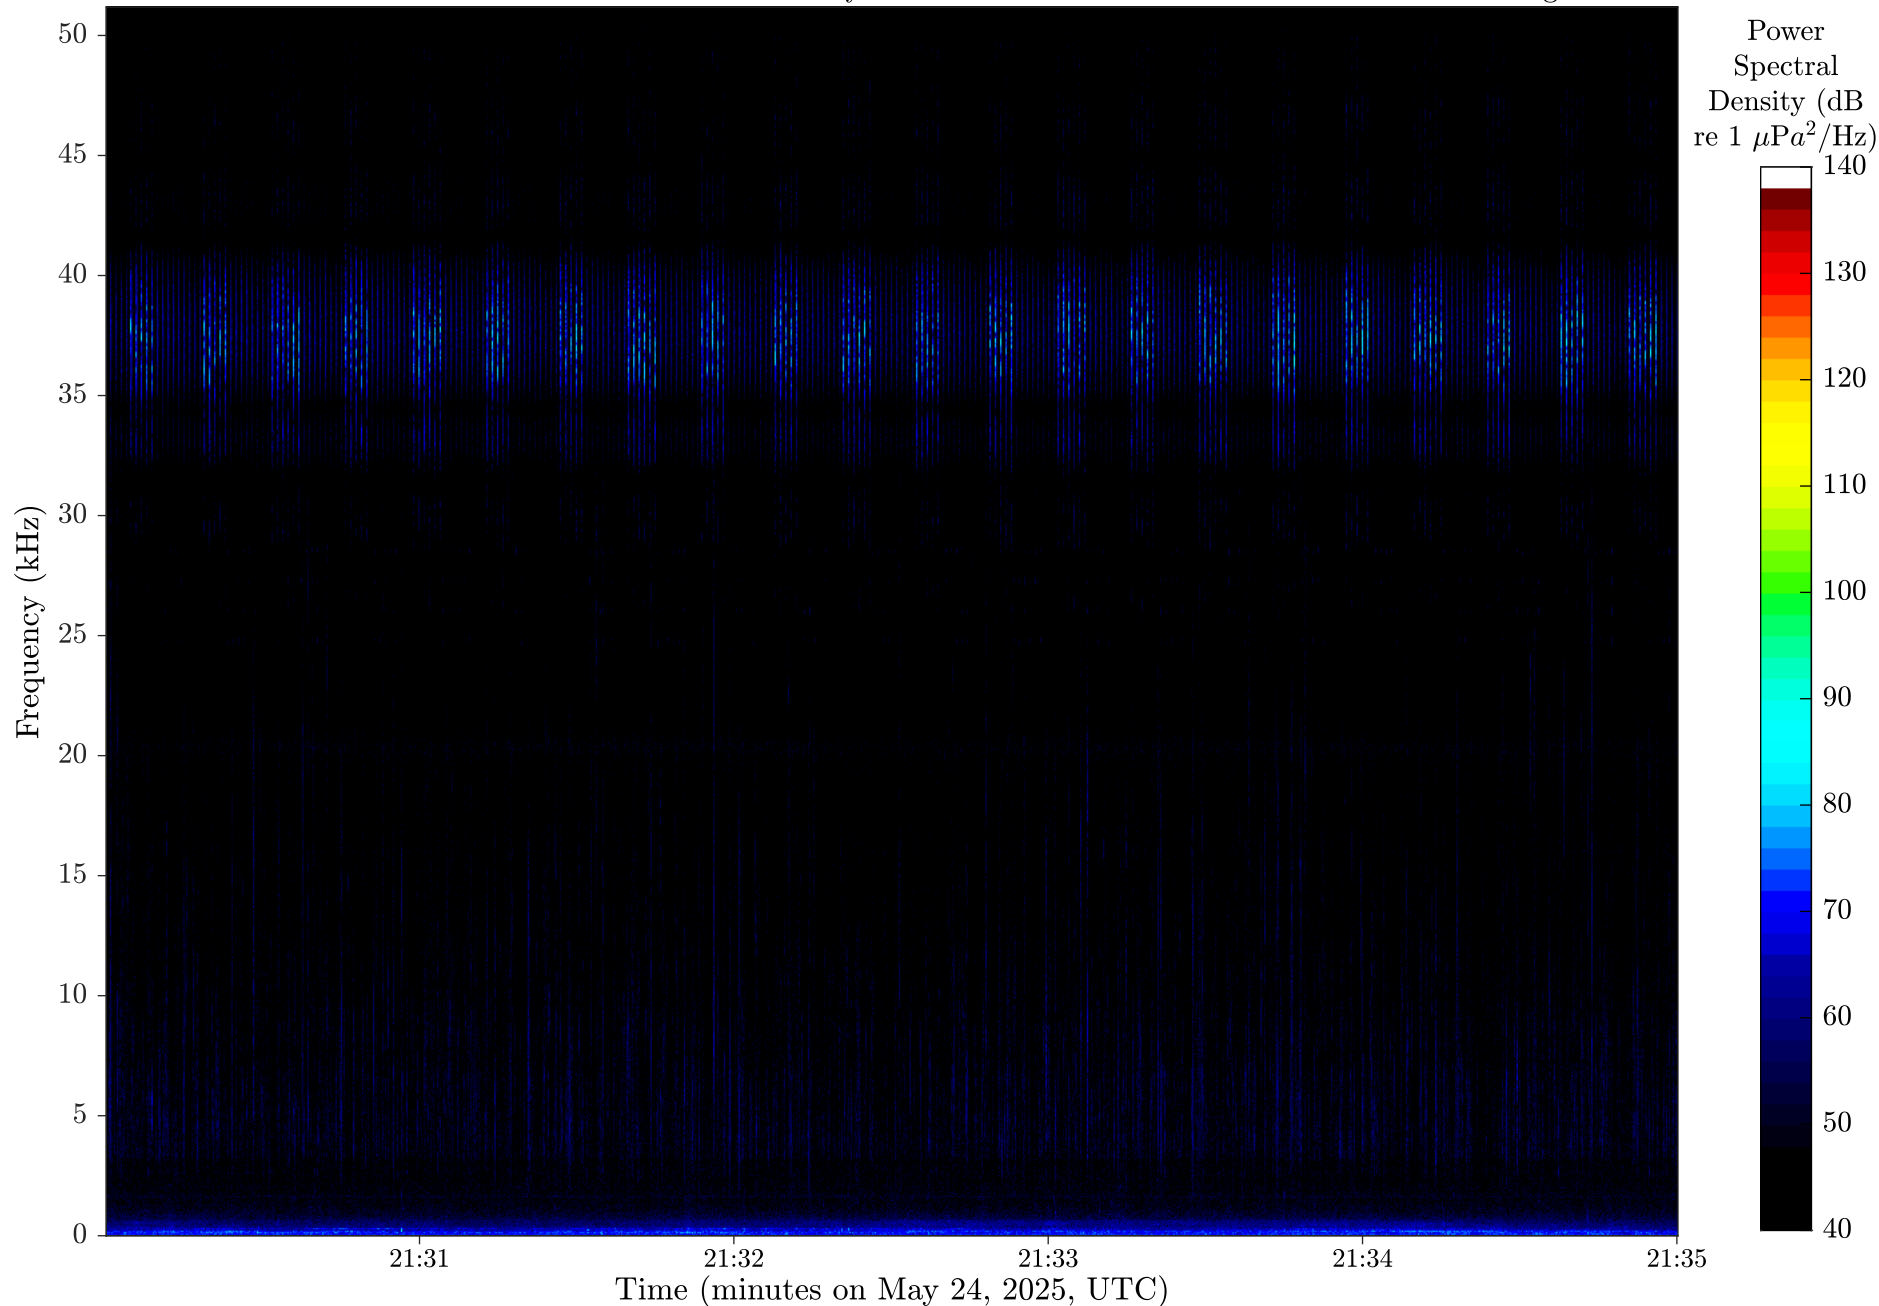

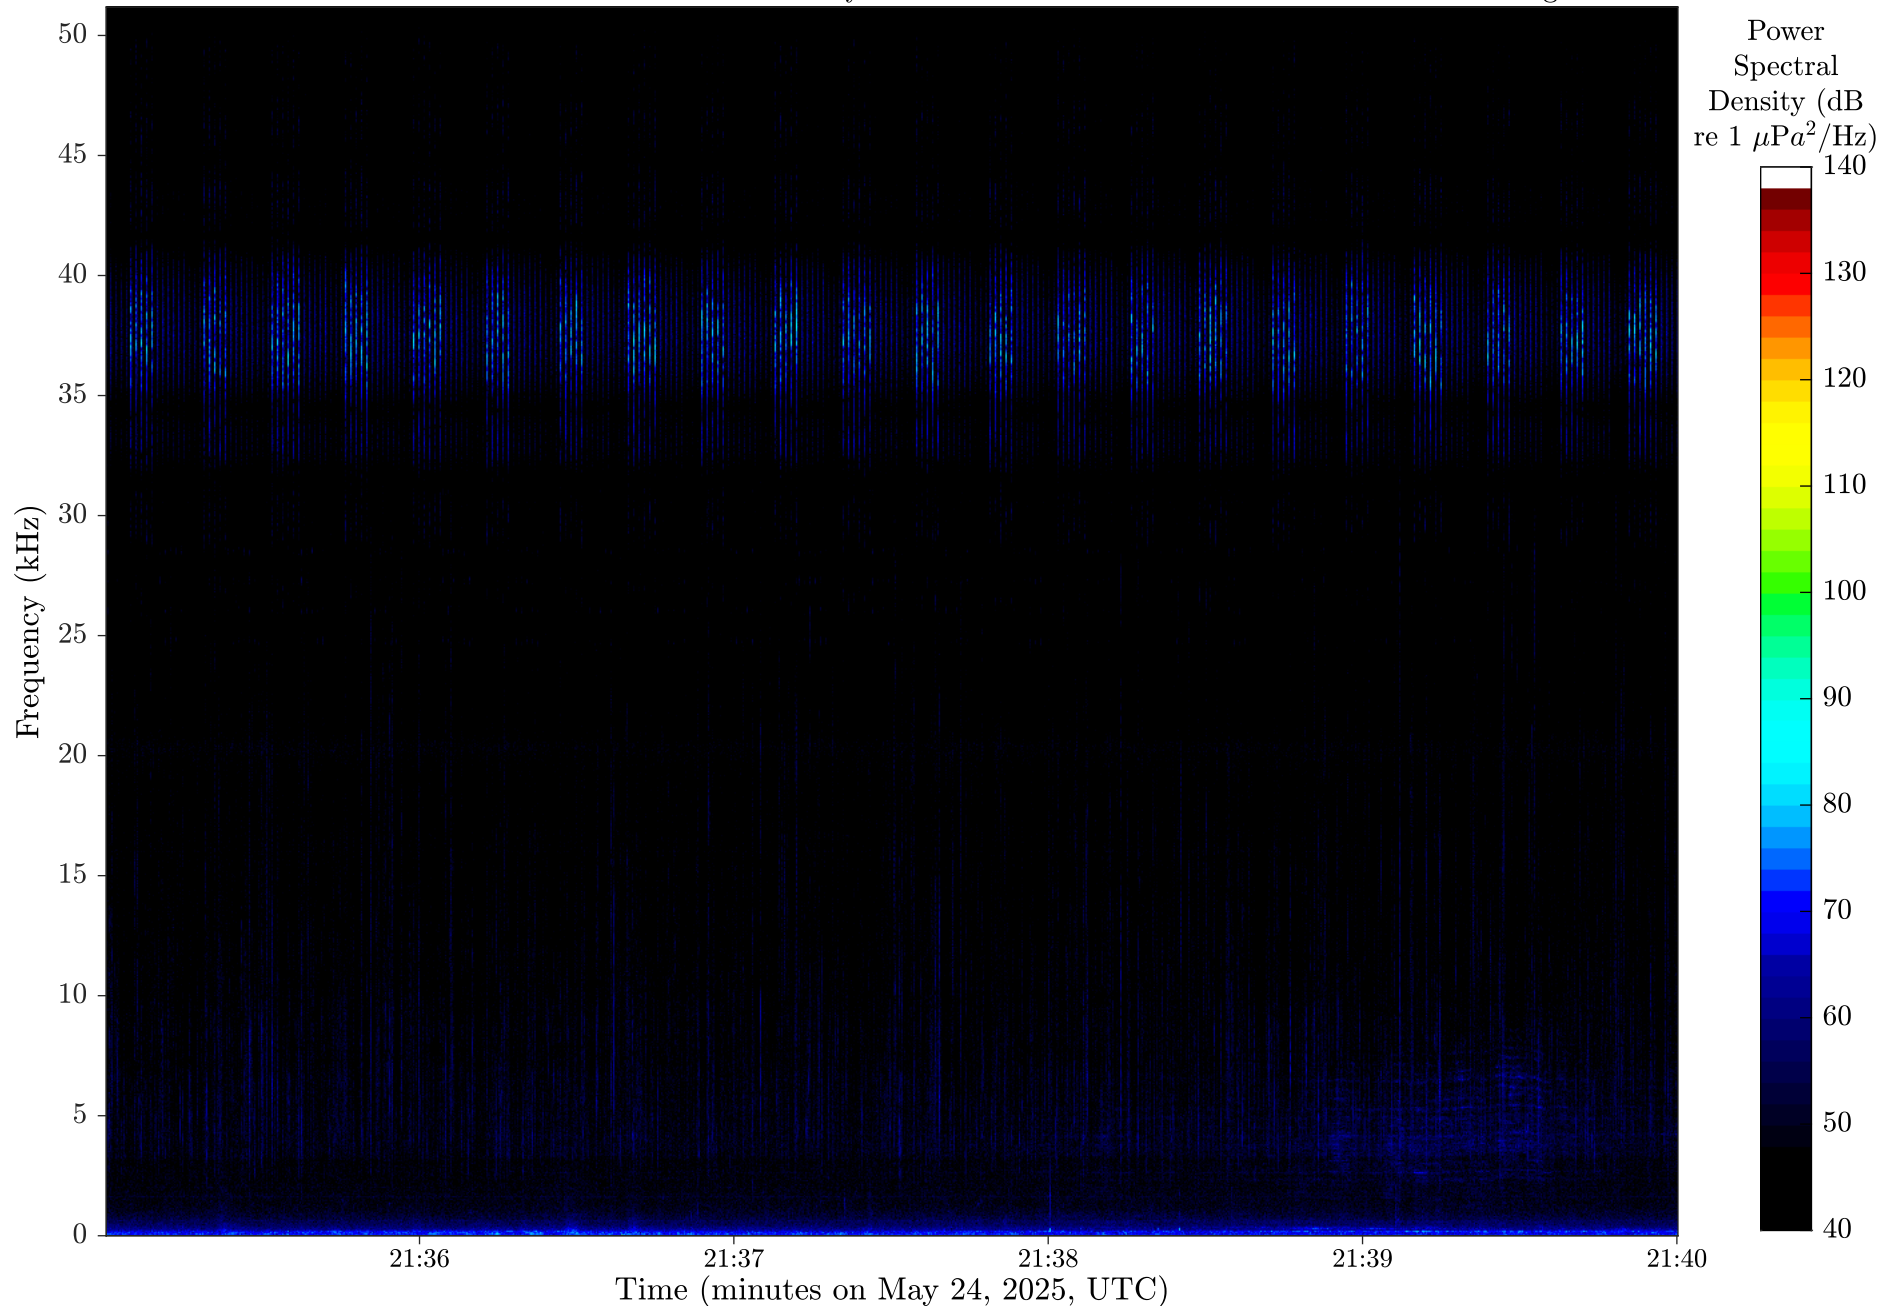


Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:50:54 UTC

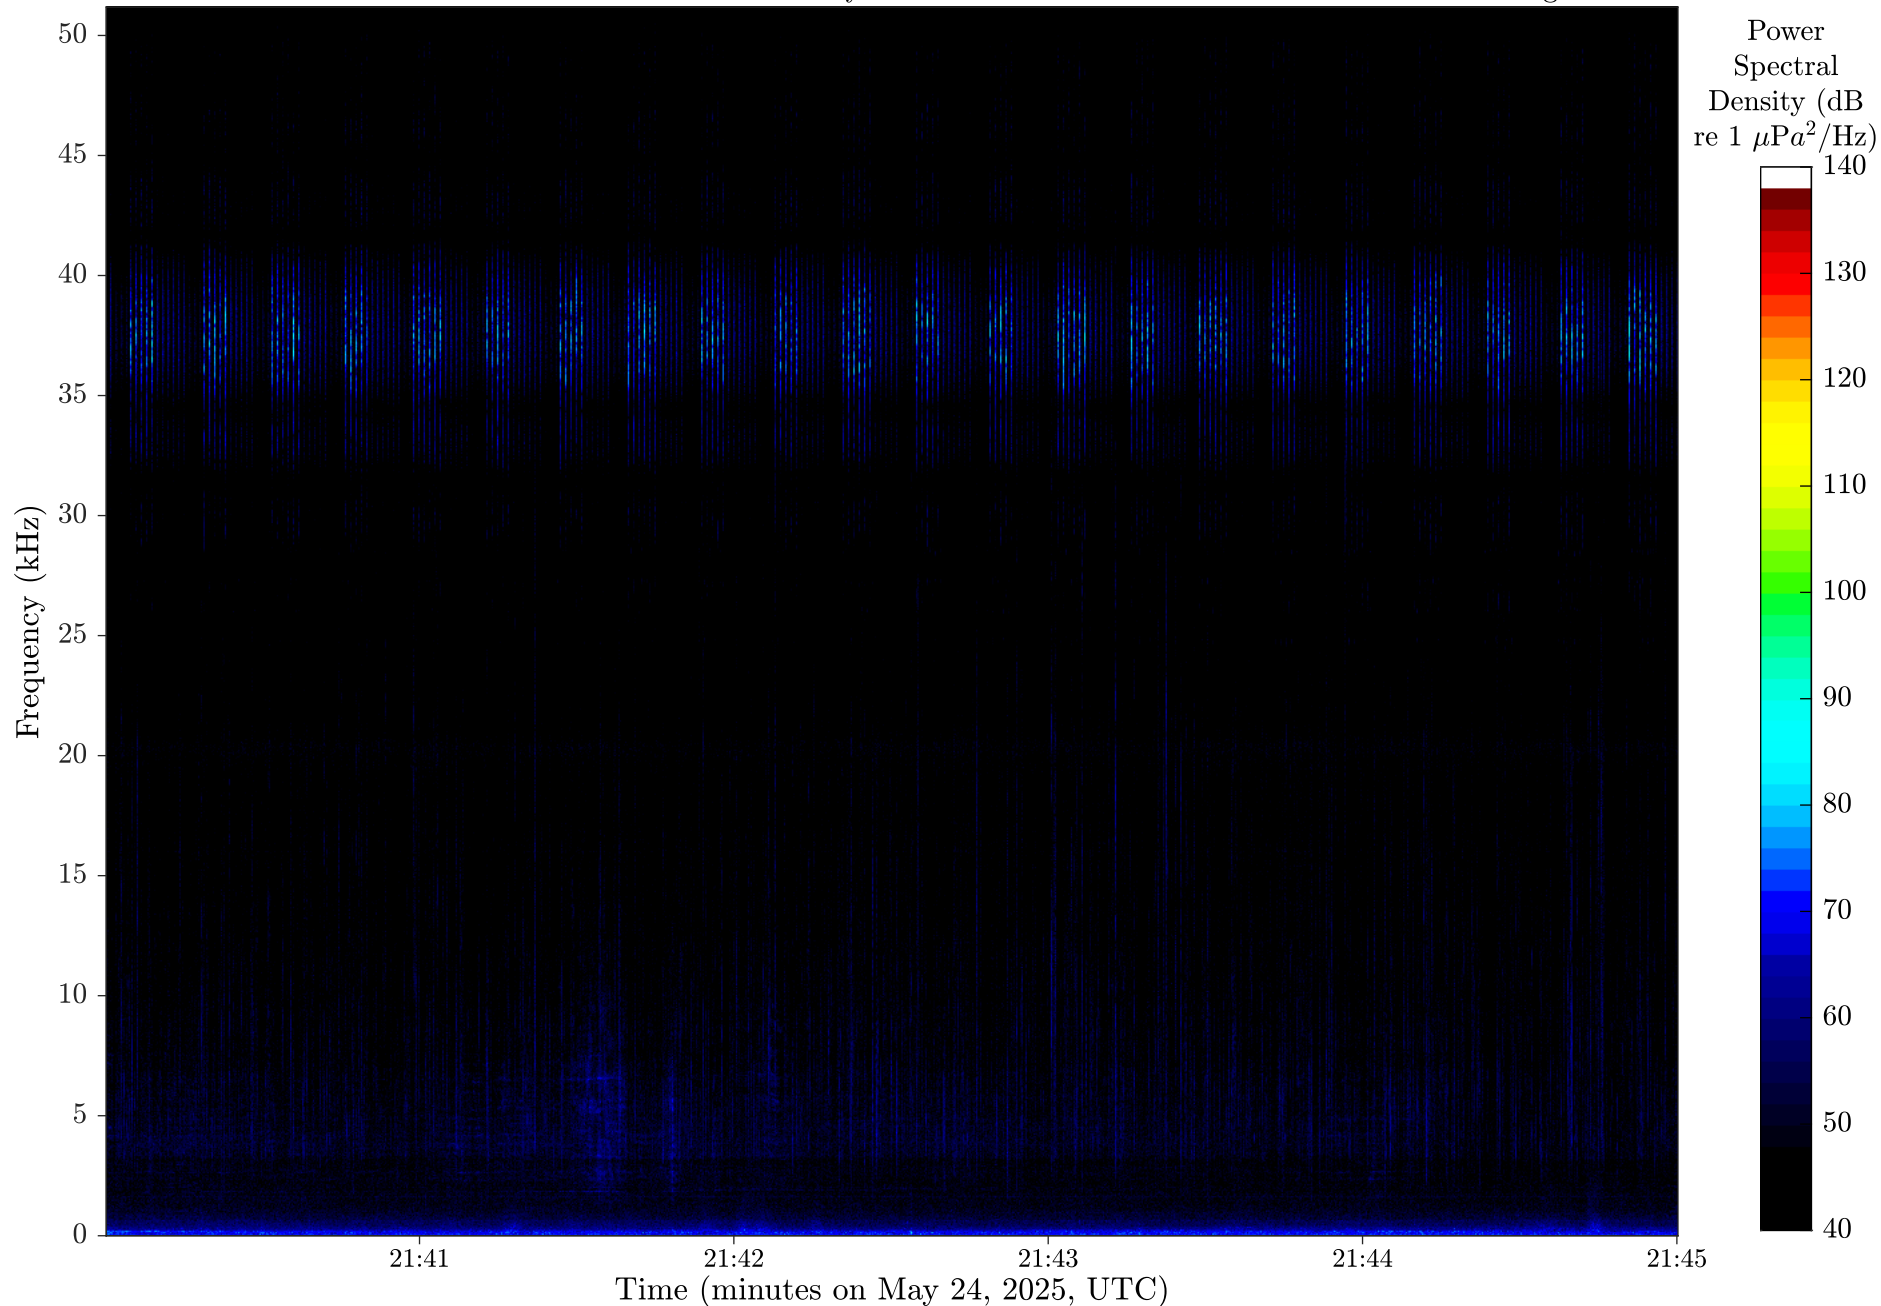

Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:51:03 UTC

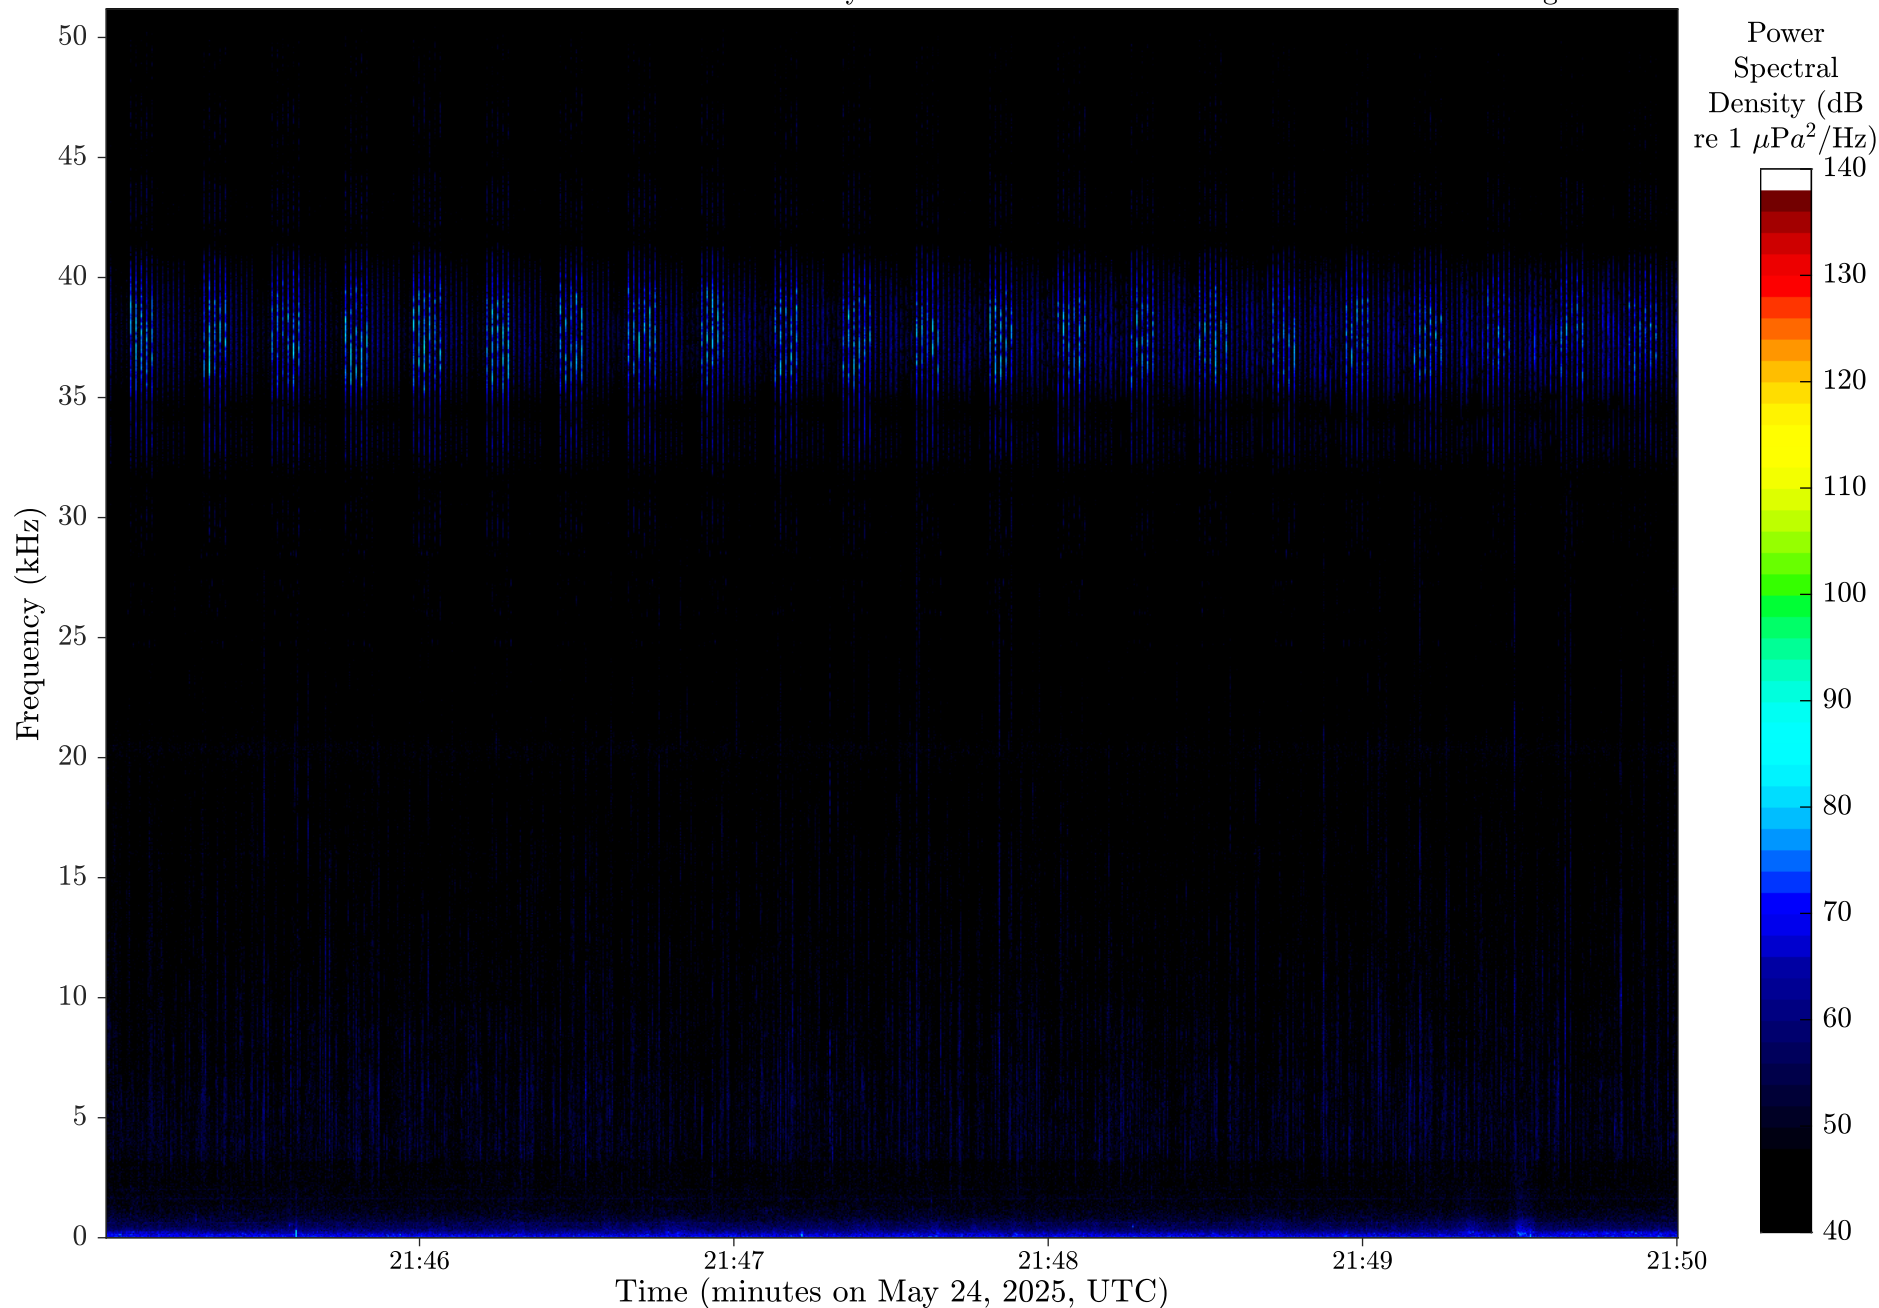

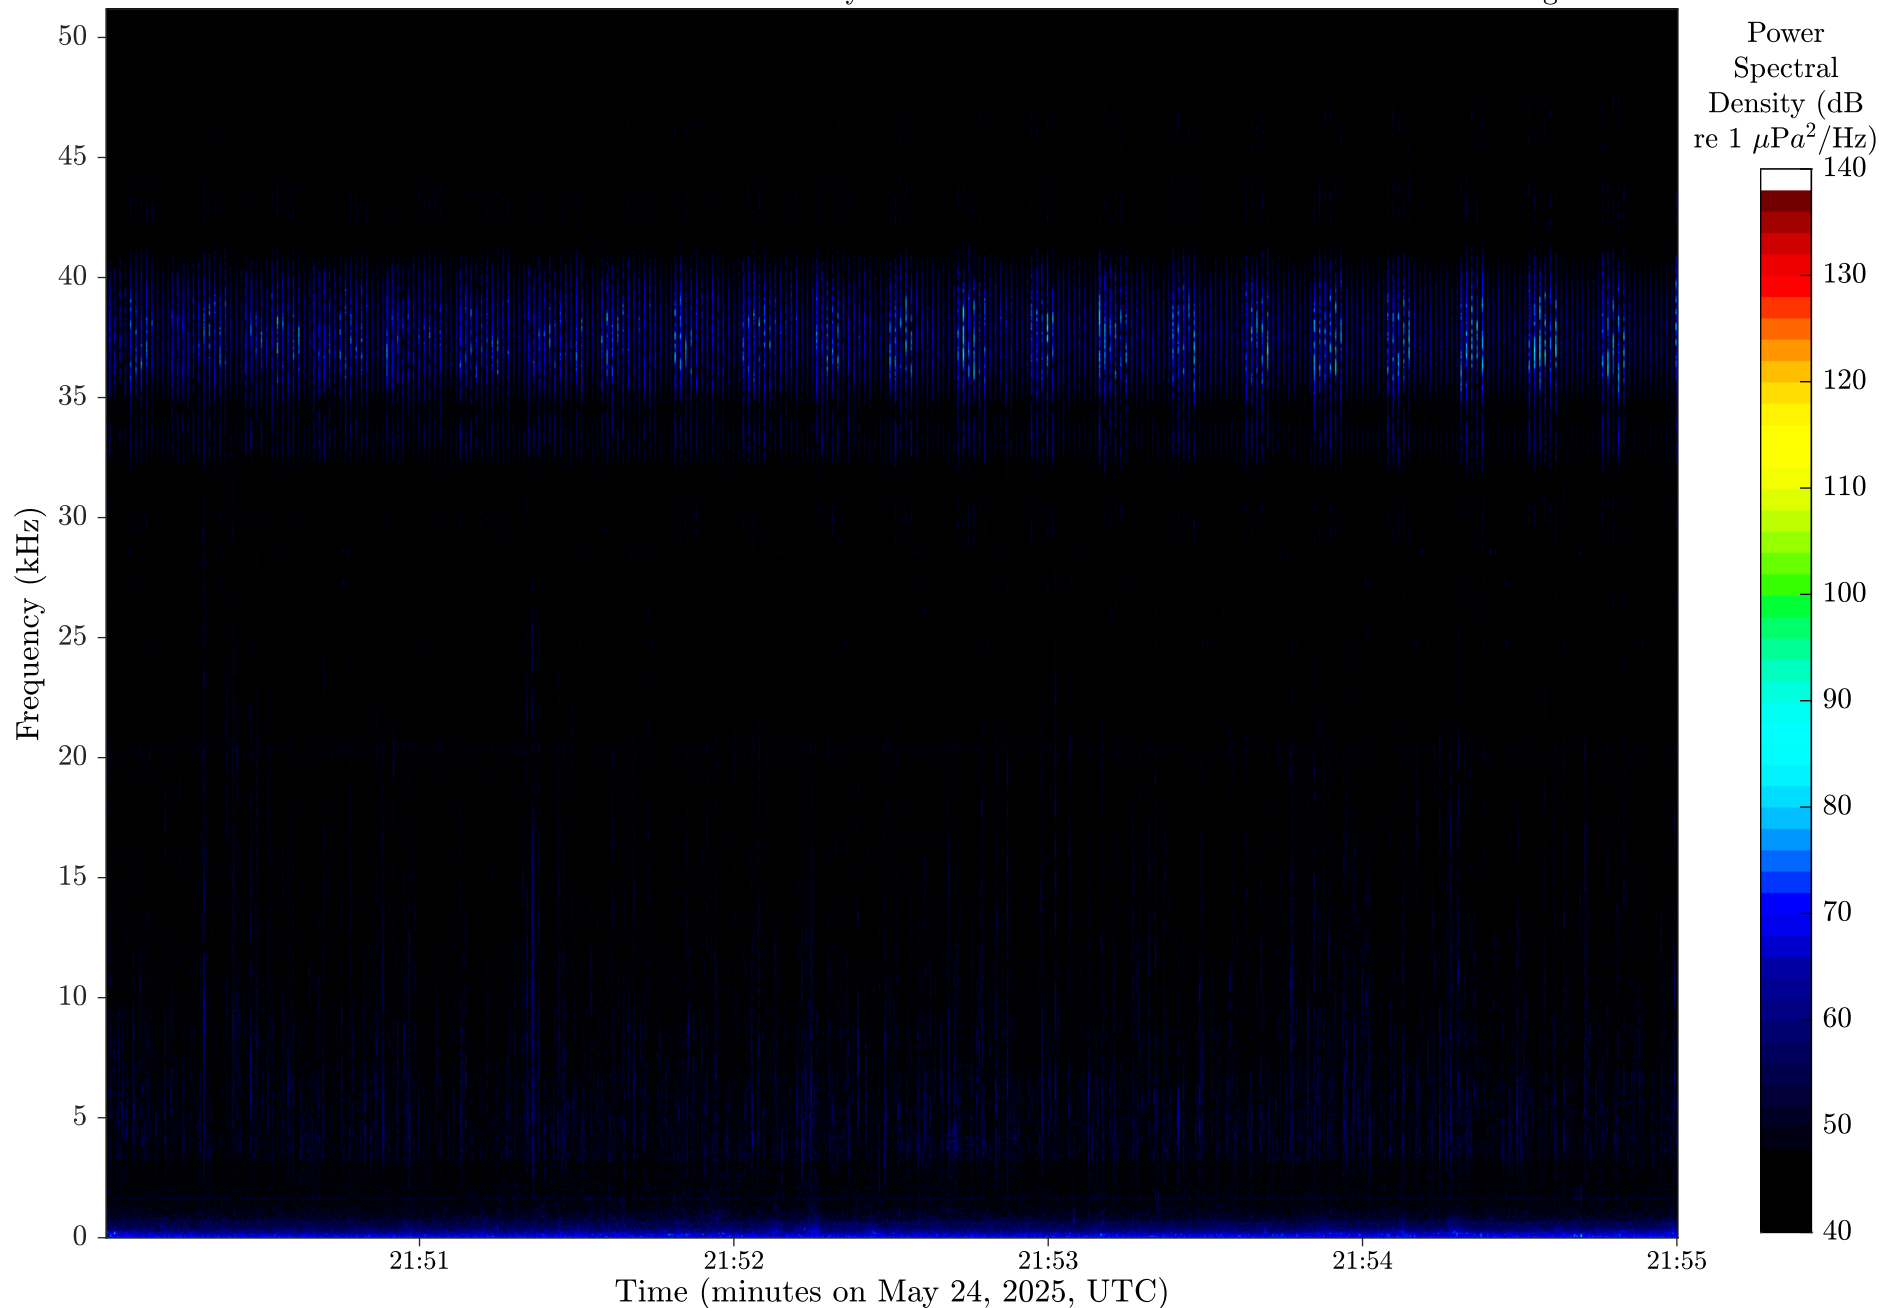


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:51:21 UTC

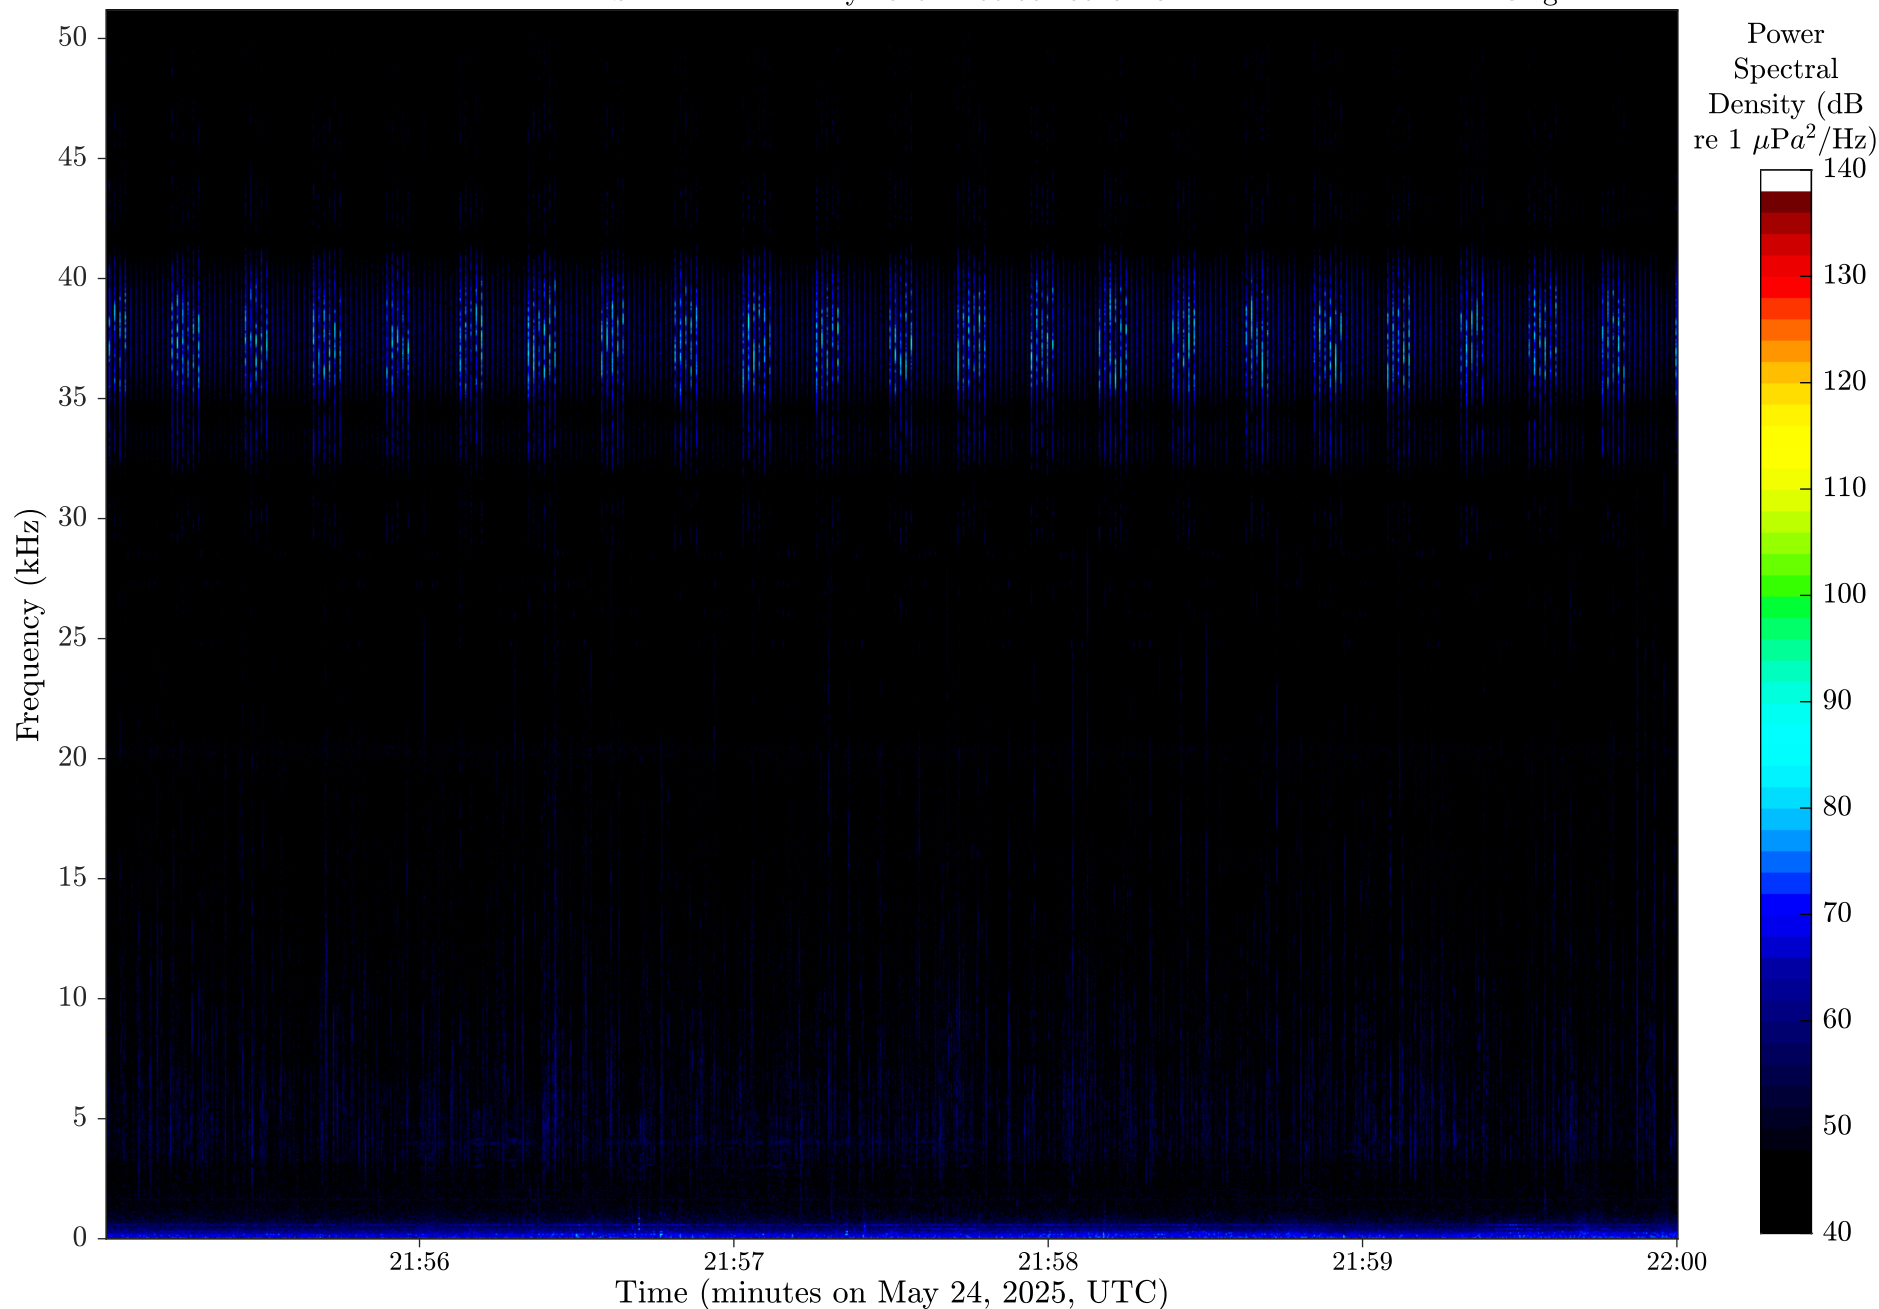


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:51:30 UTC

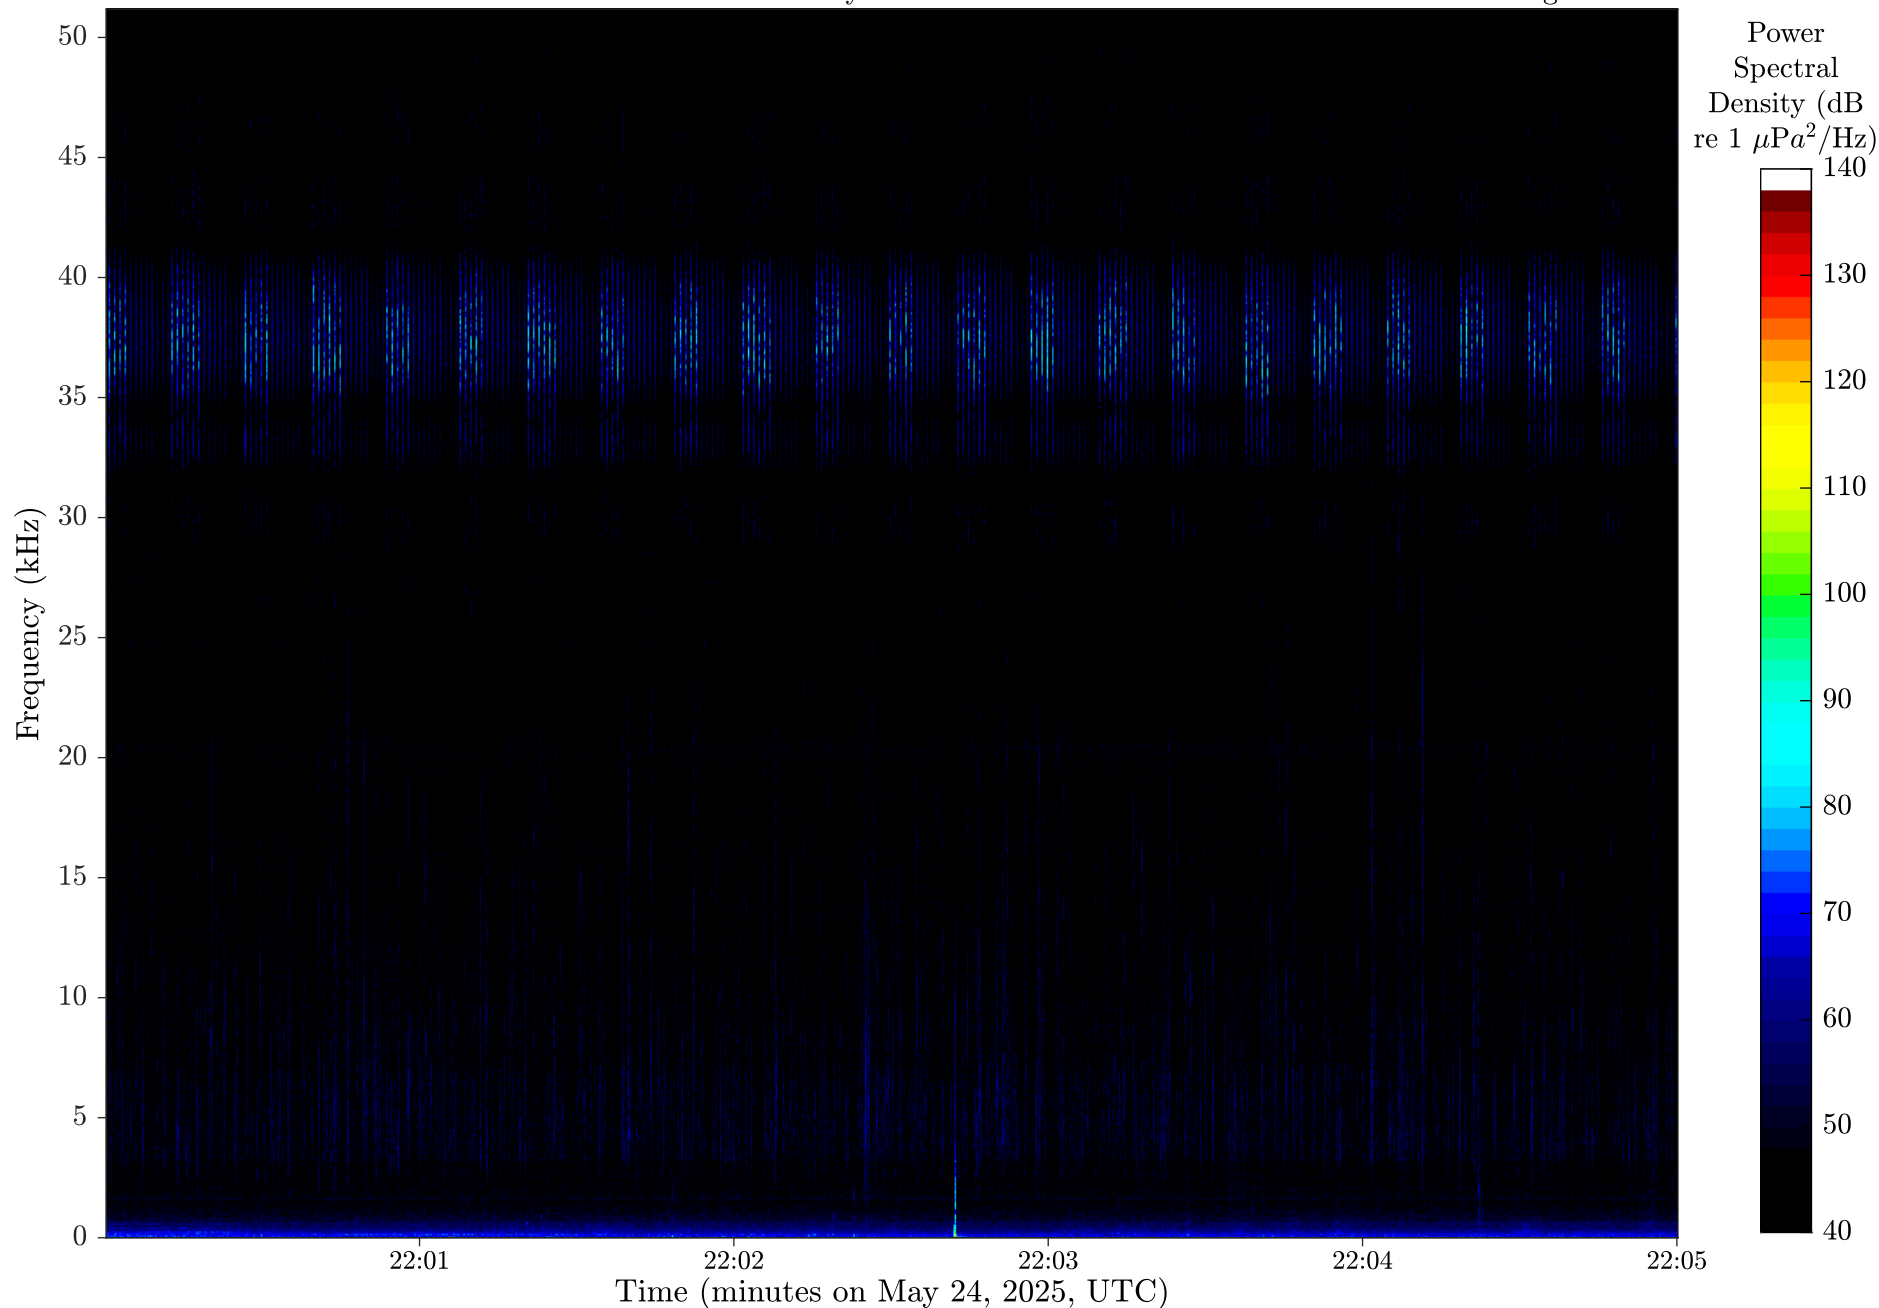



Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:51:38 UTC

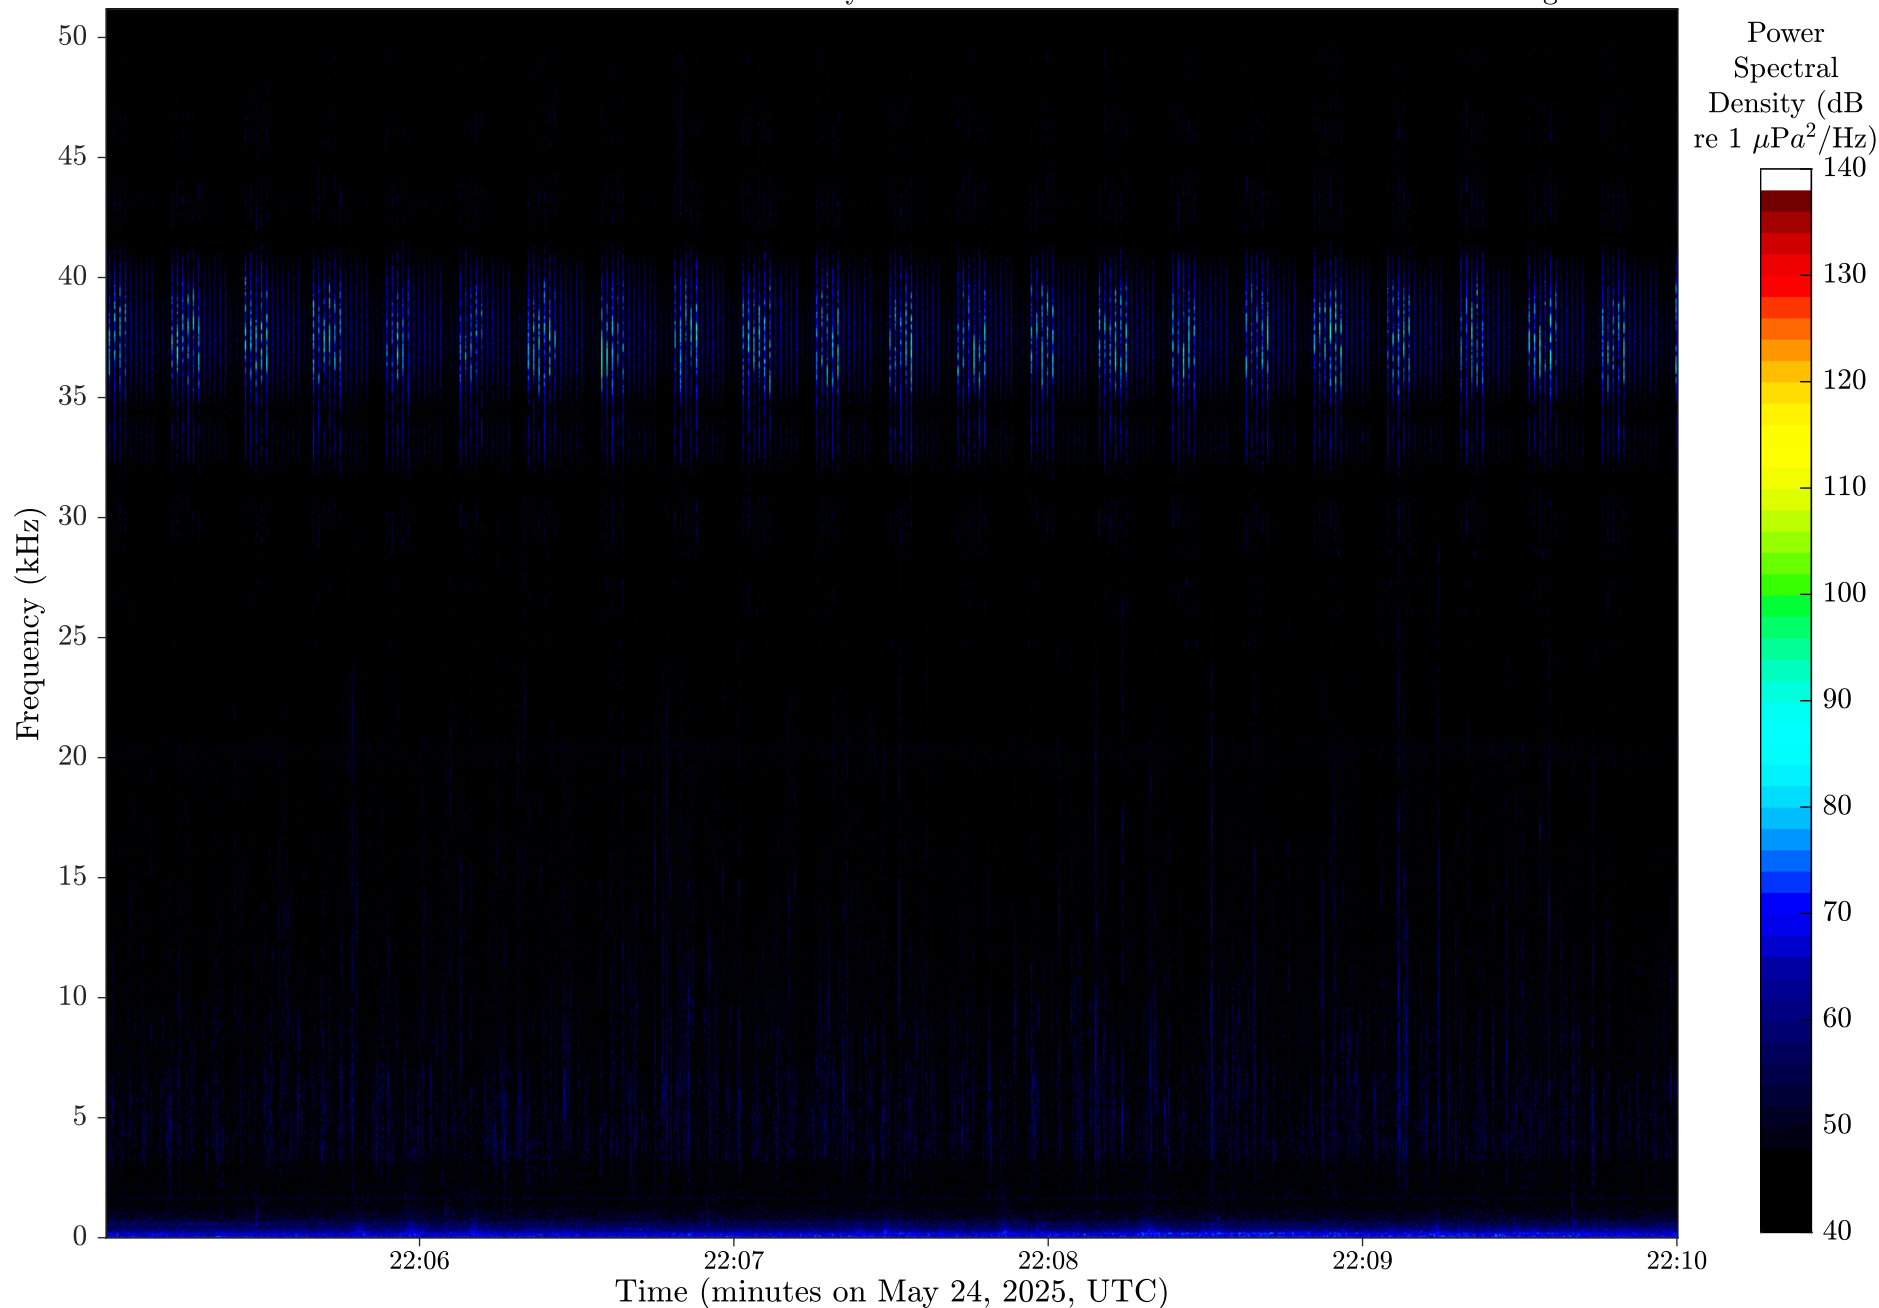

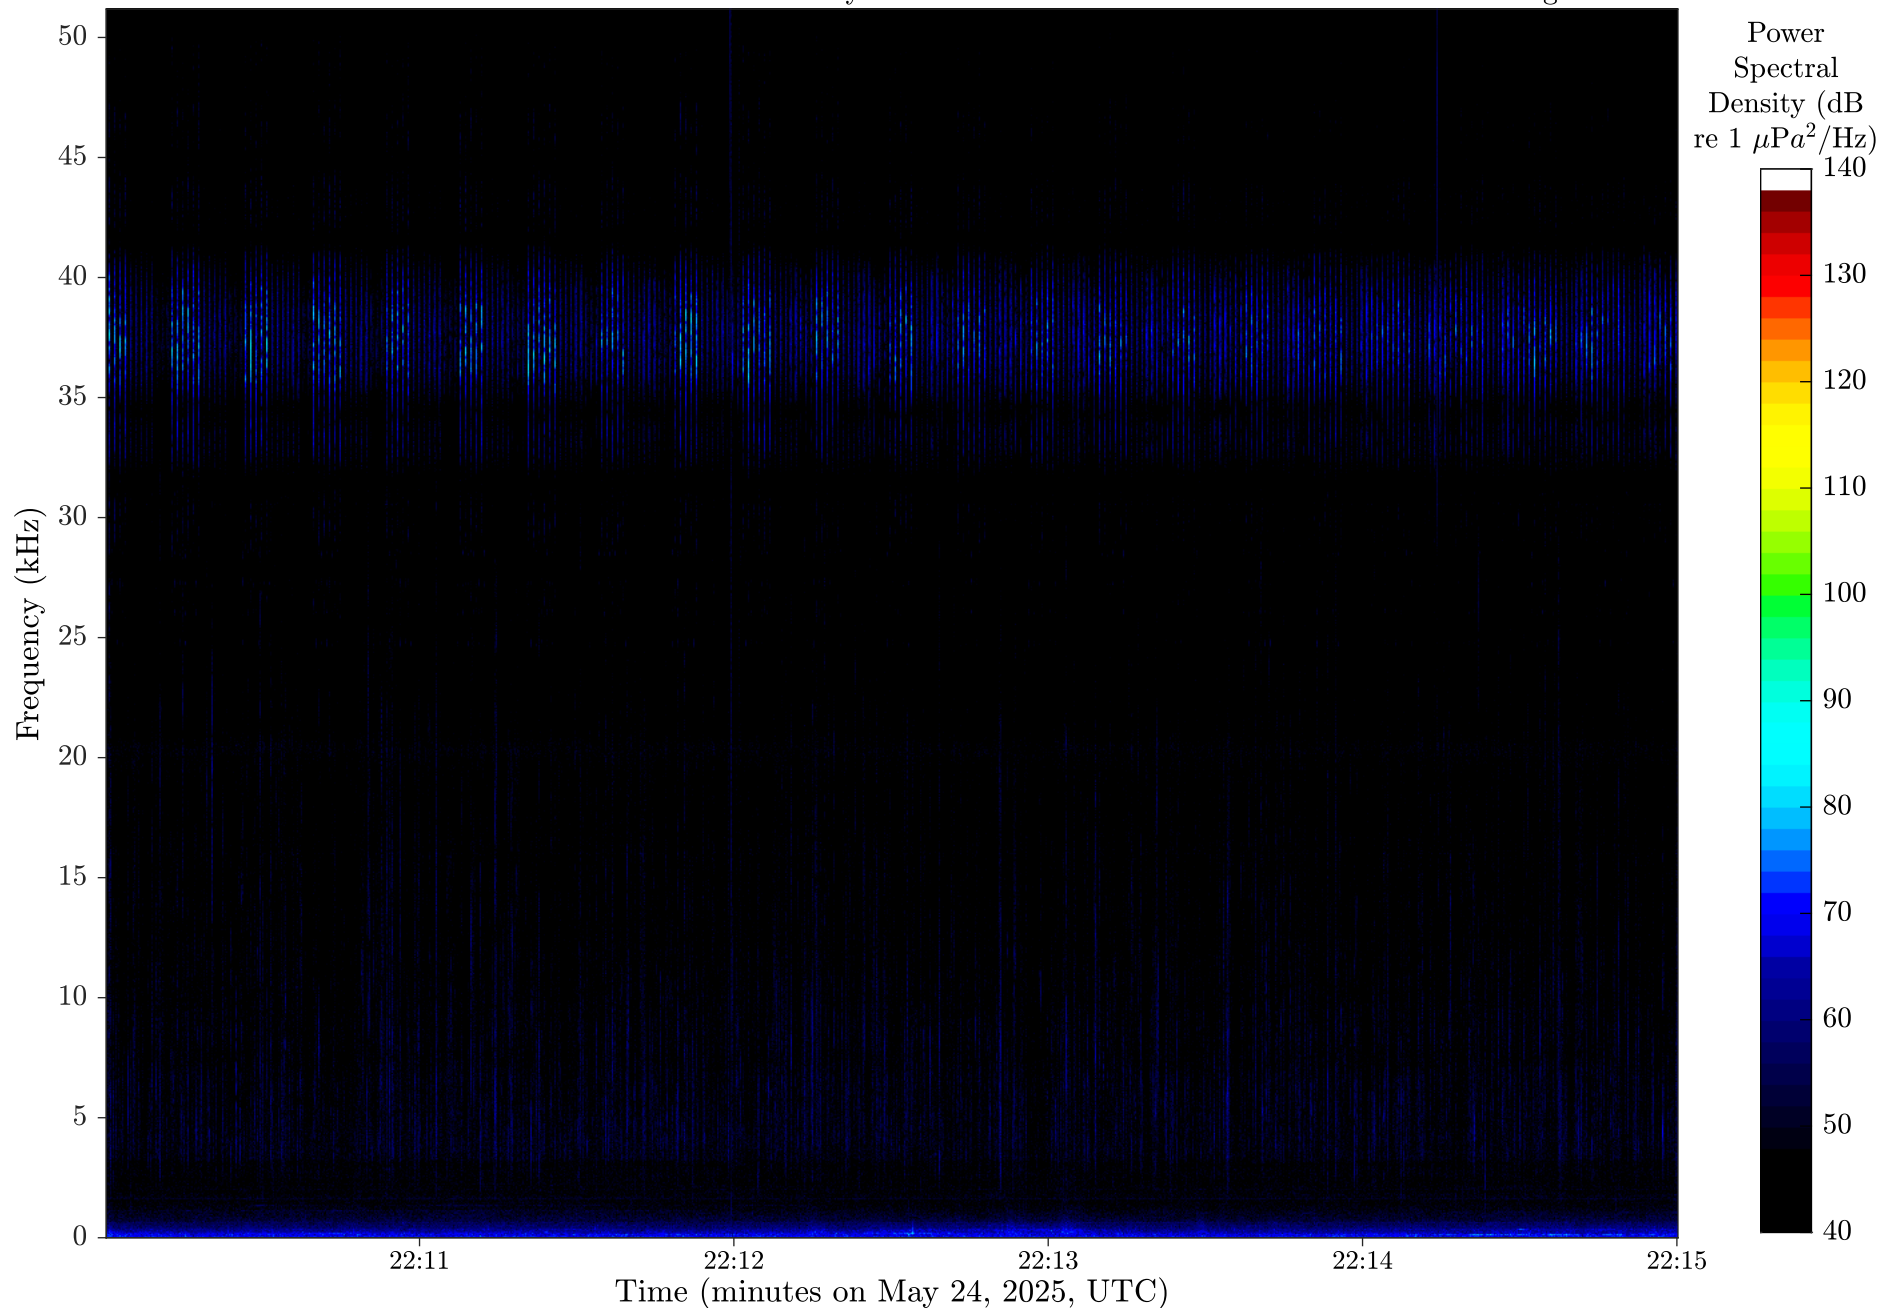


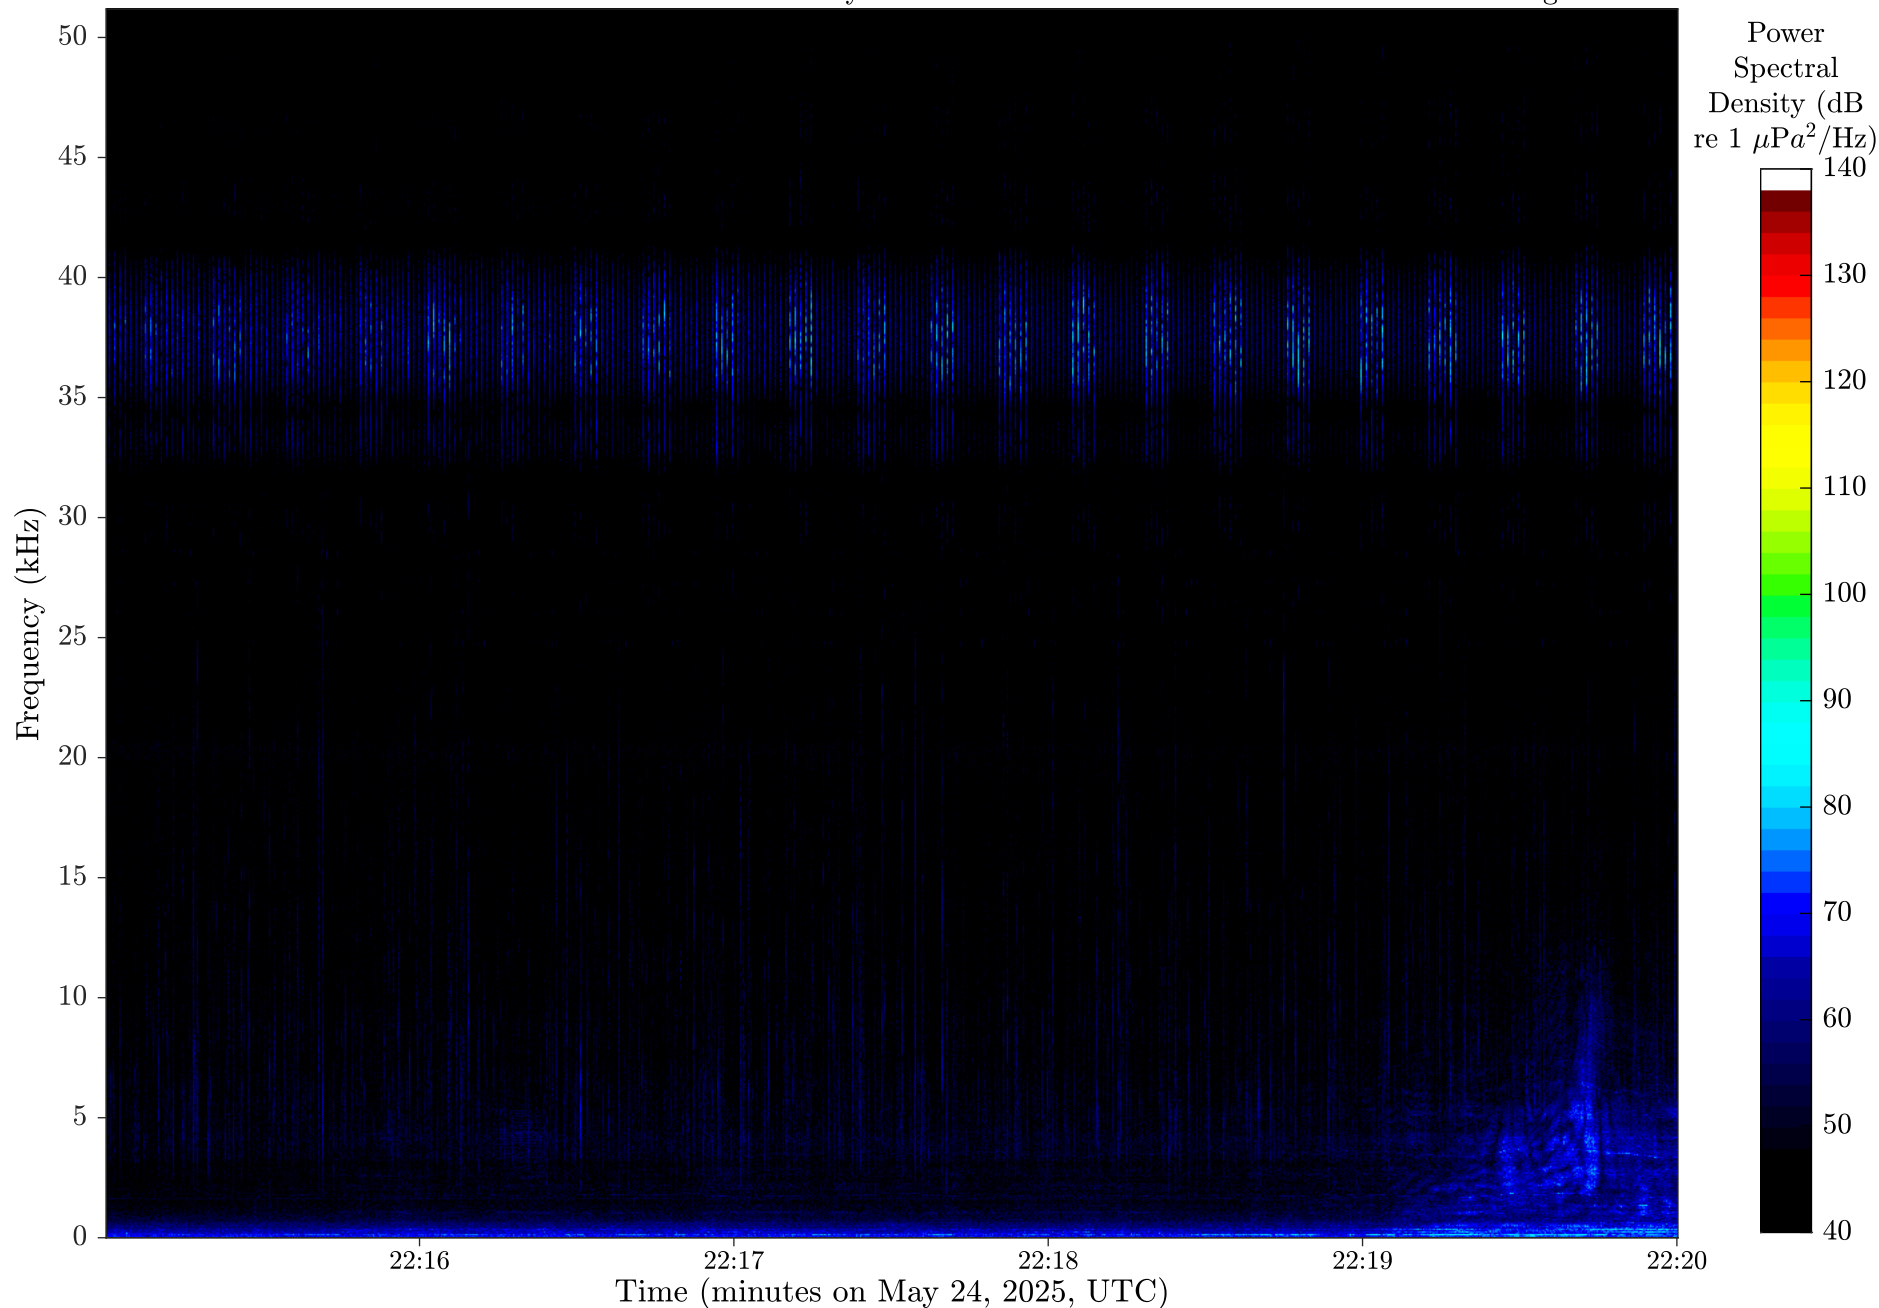

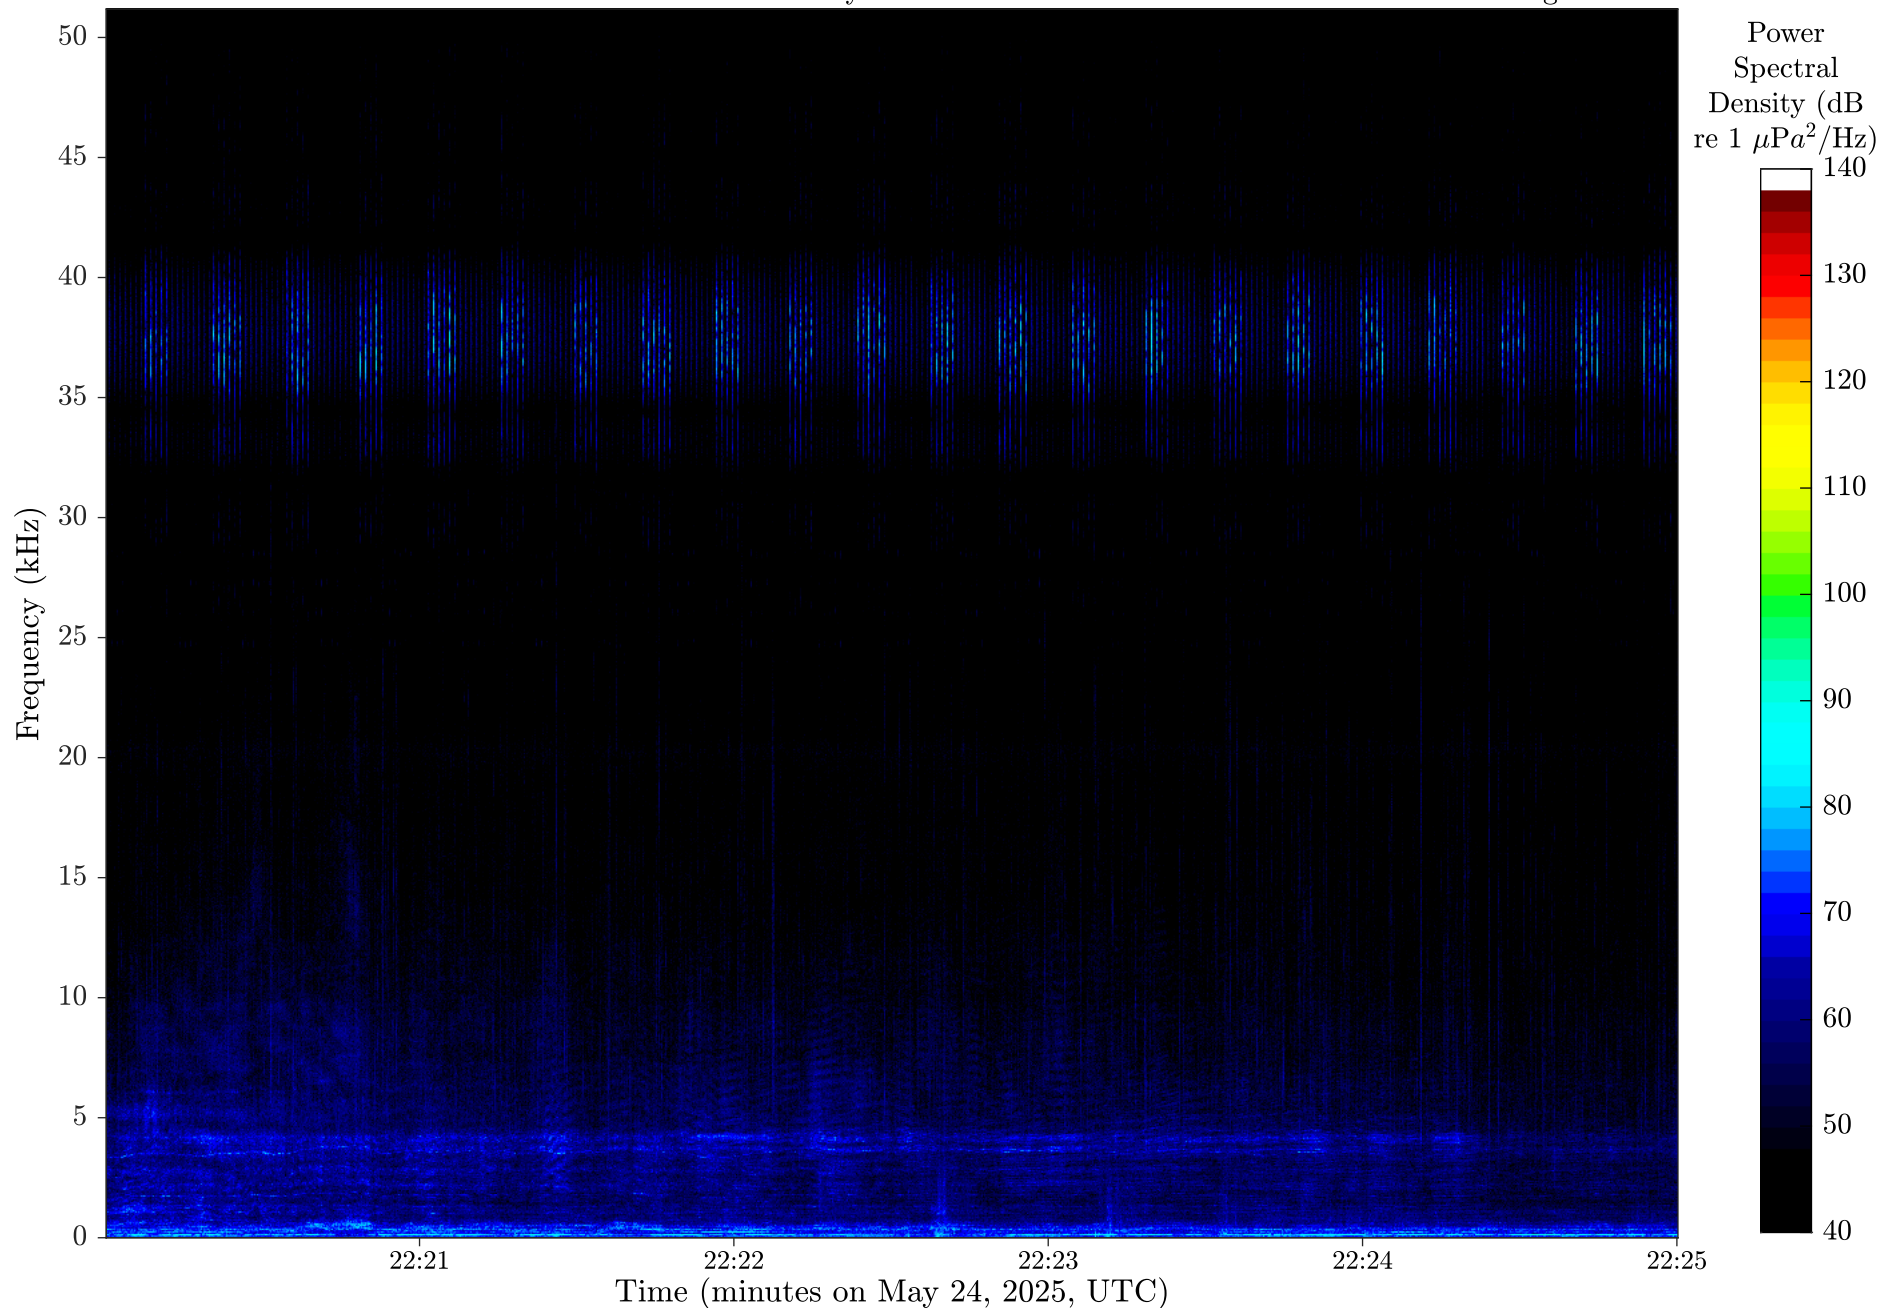


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:52:14 UTC

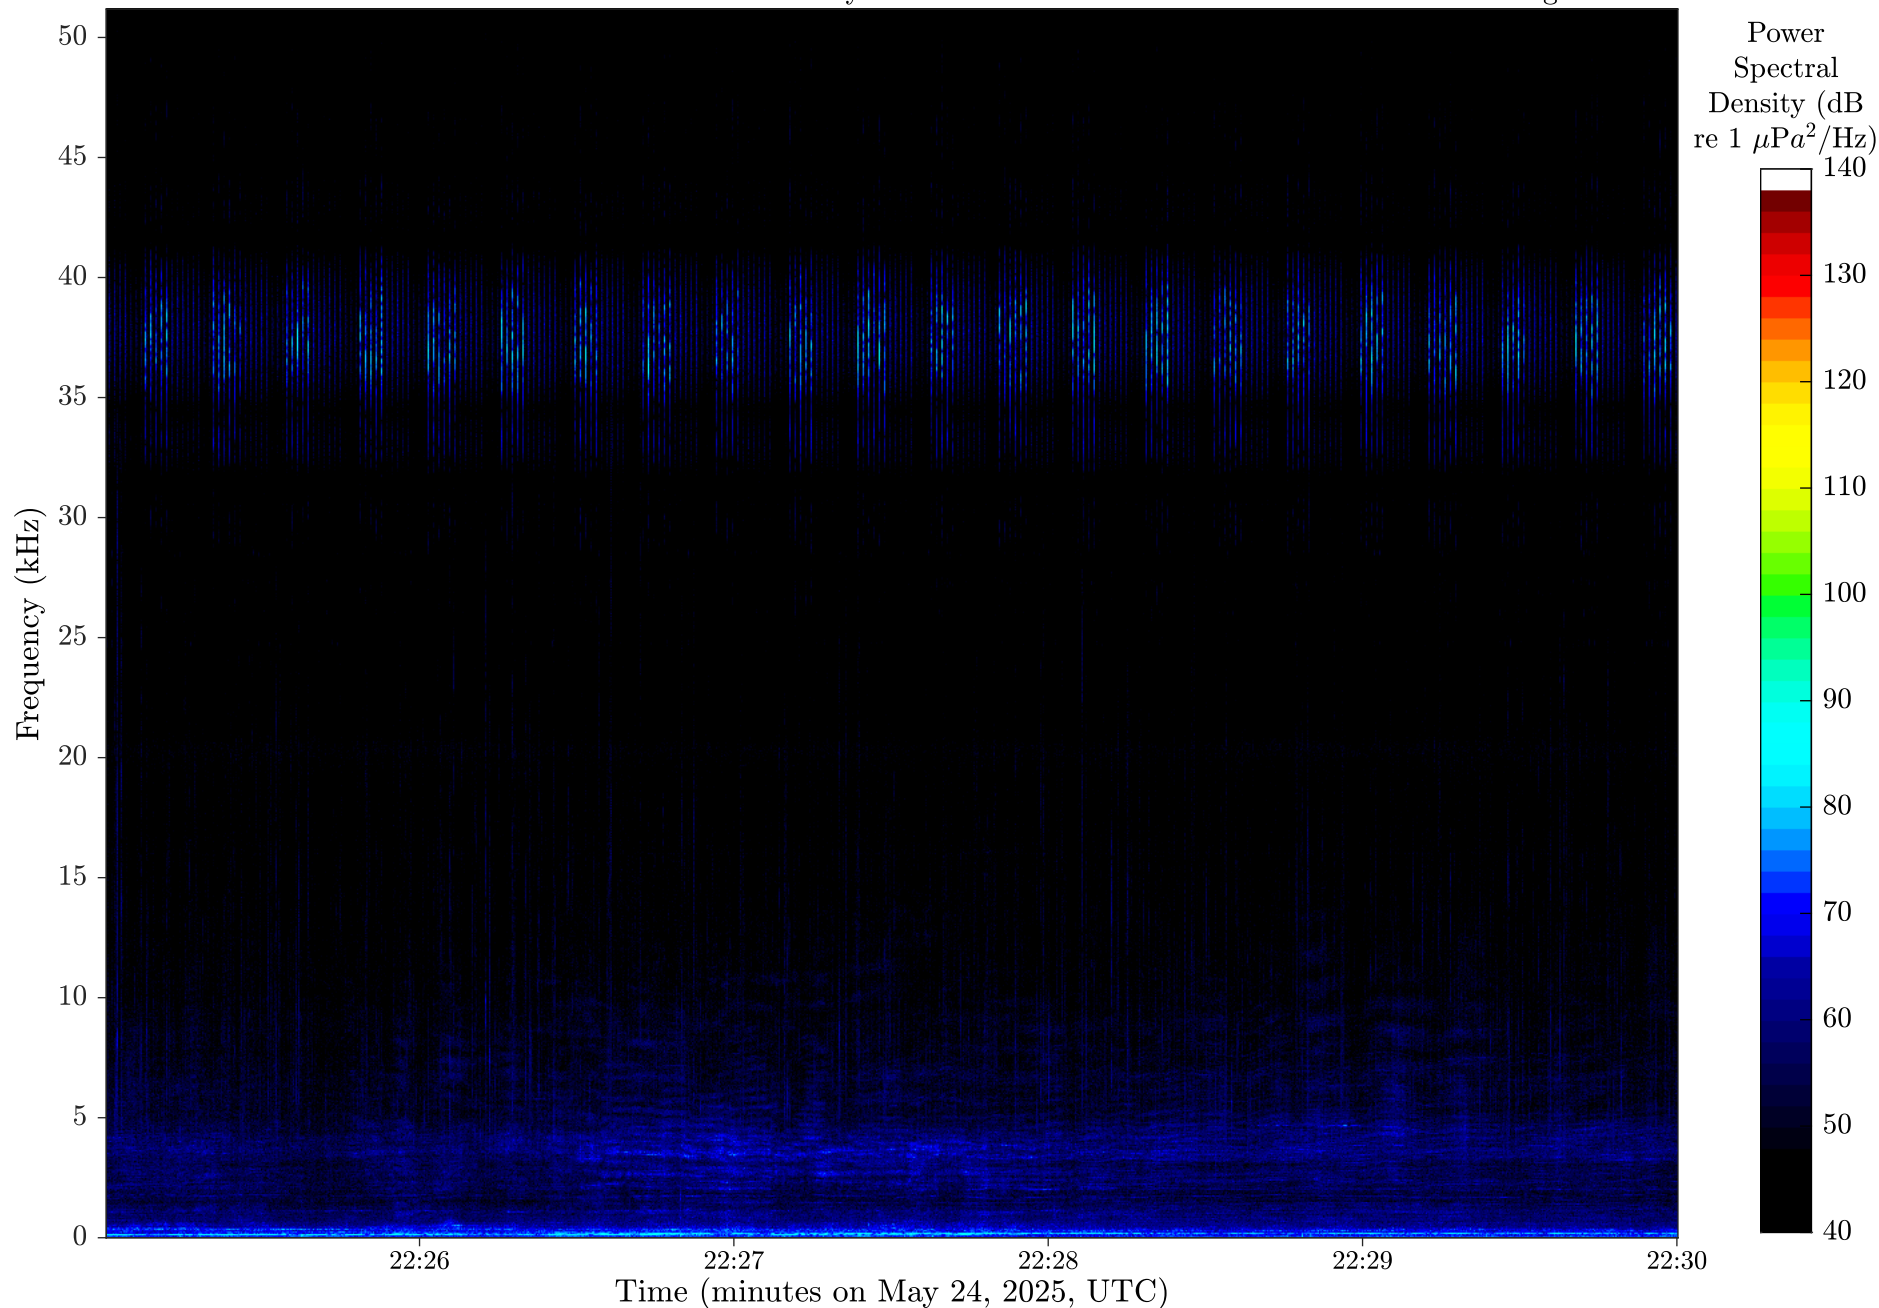


Comments: 34.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:52:23 UTC

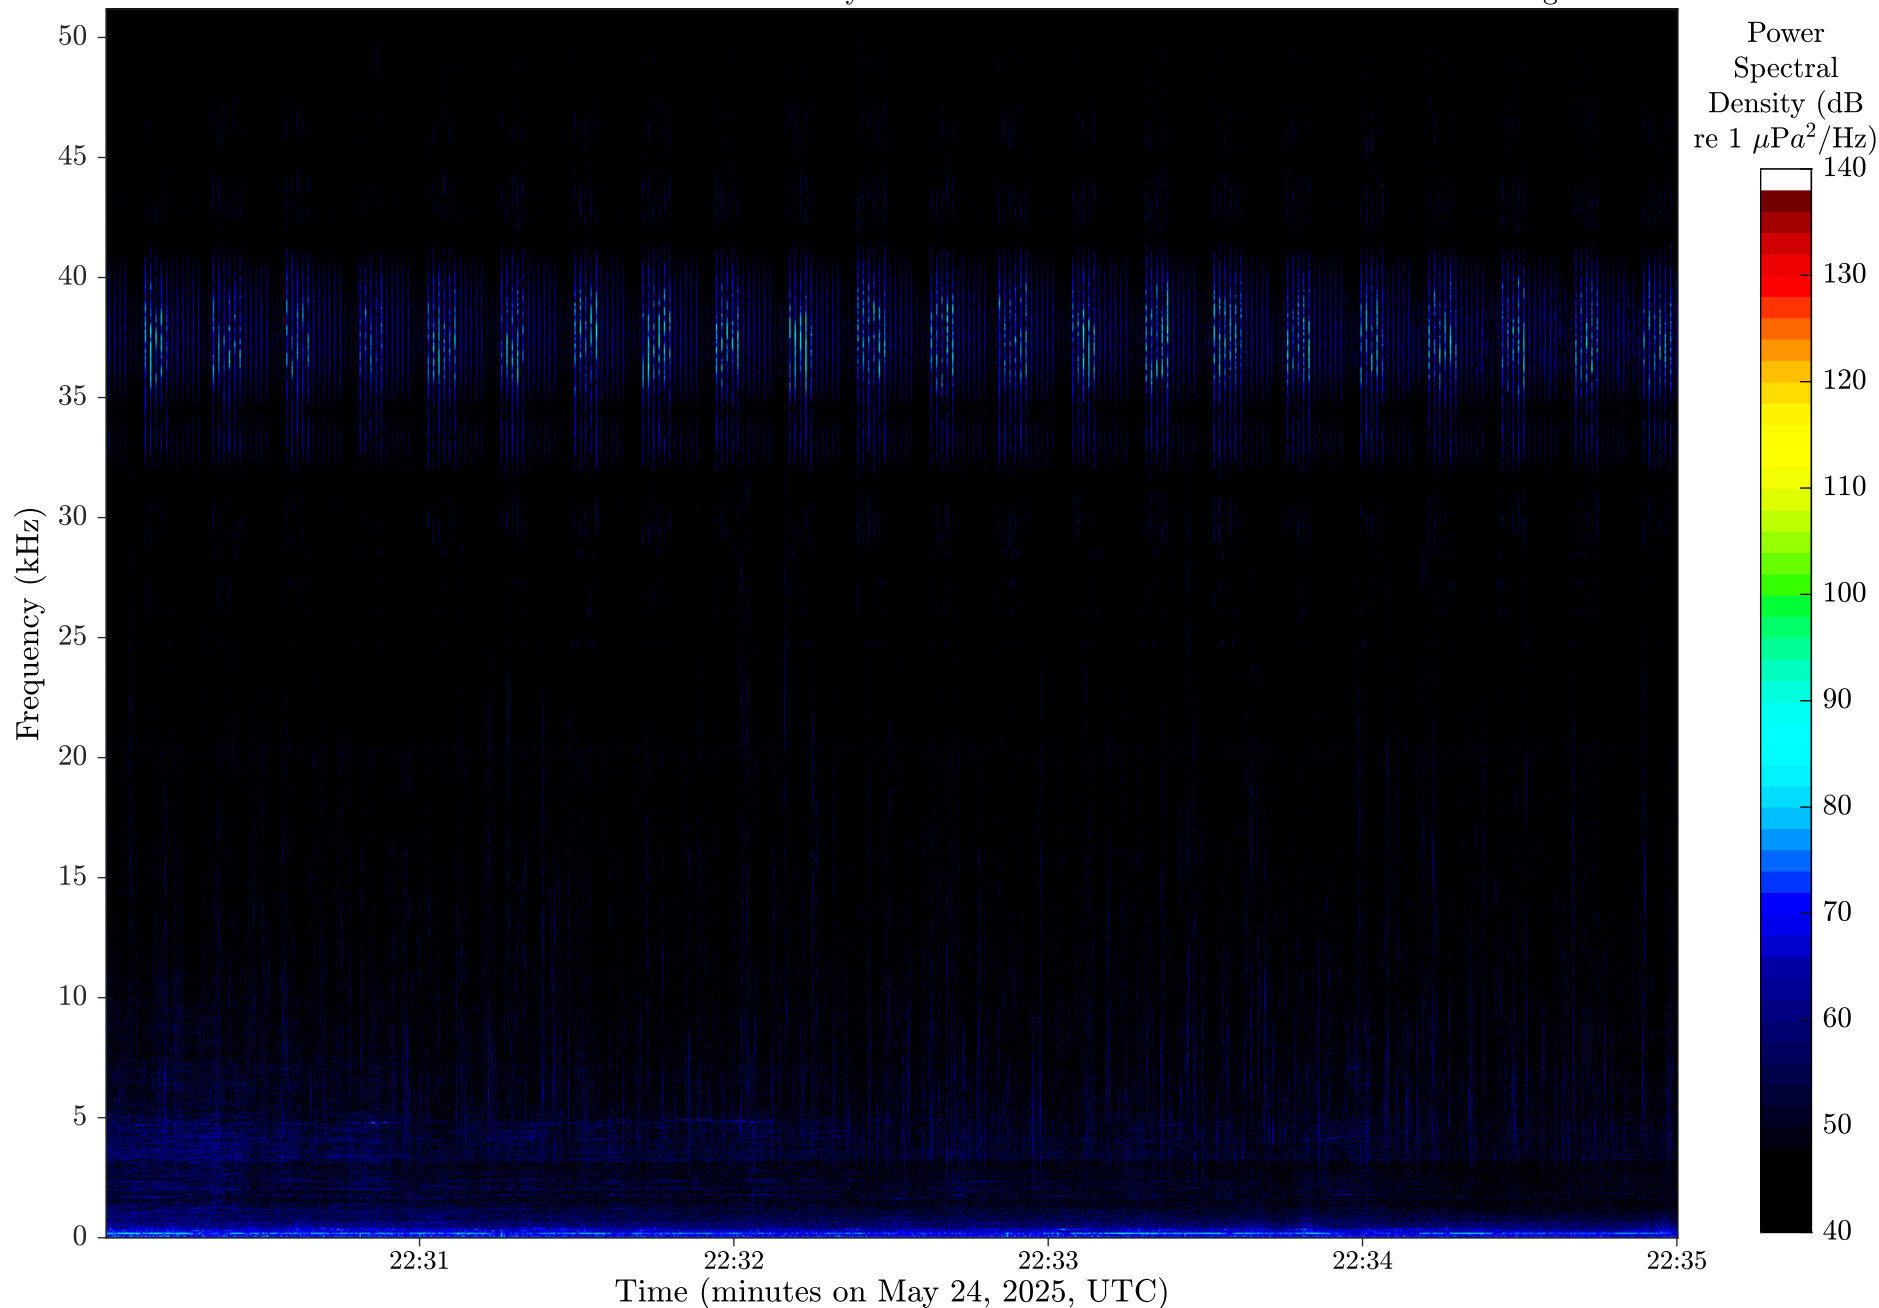


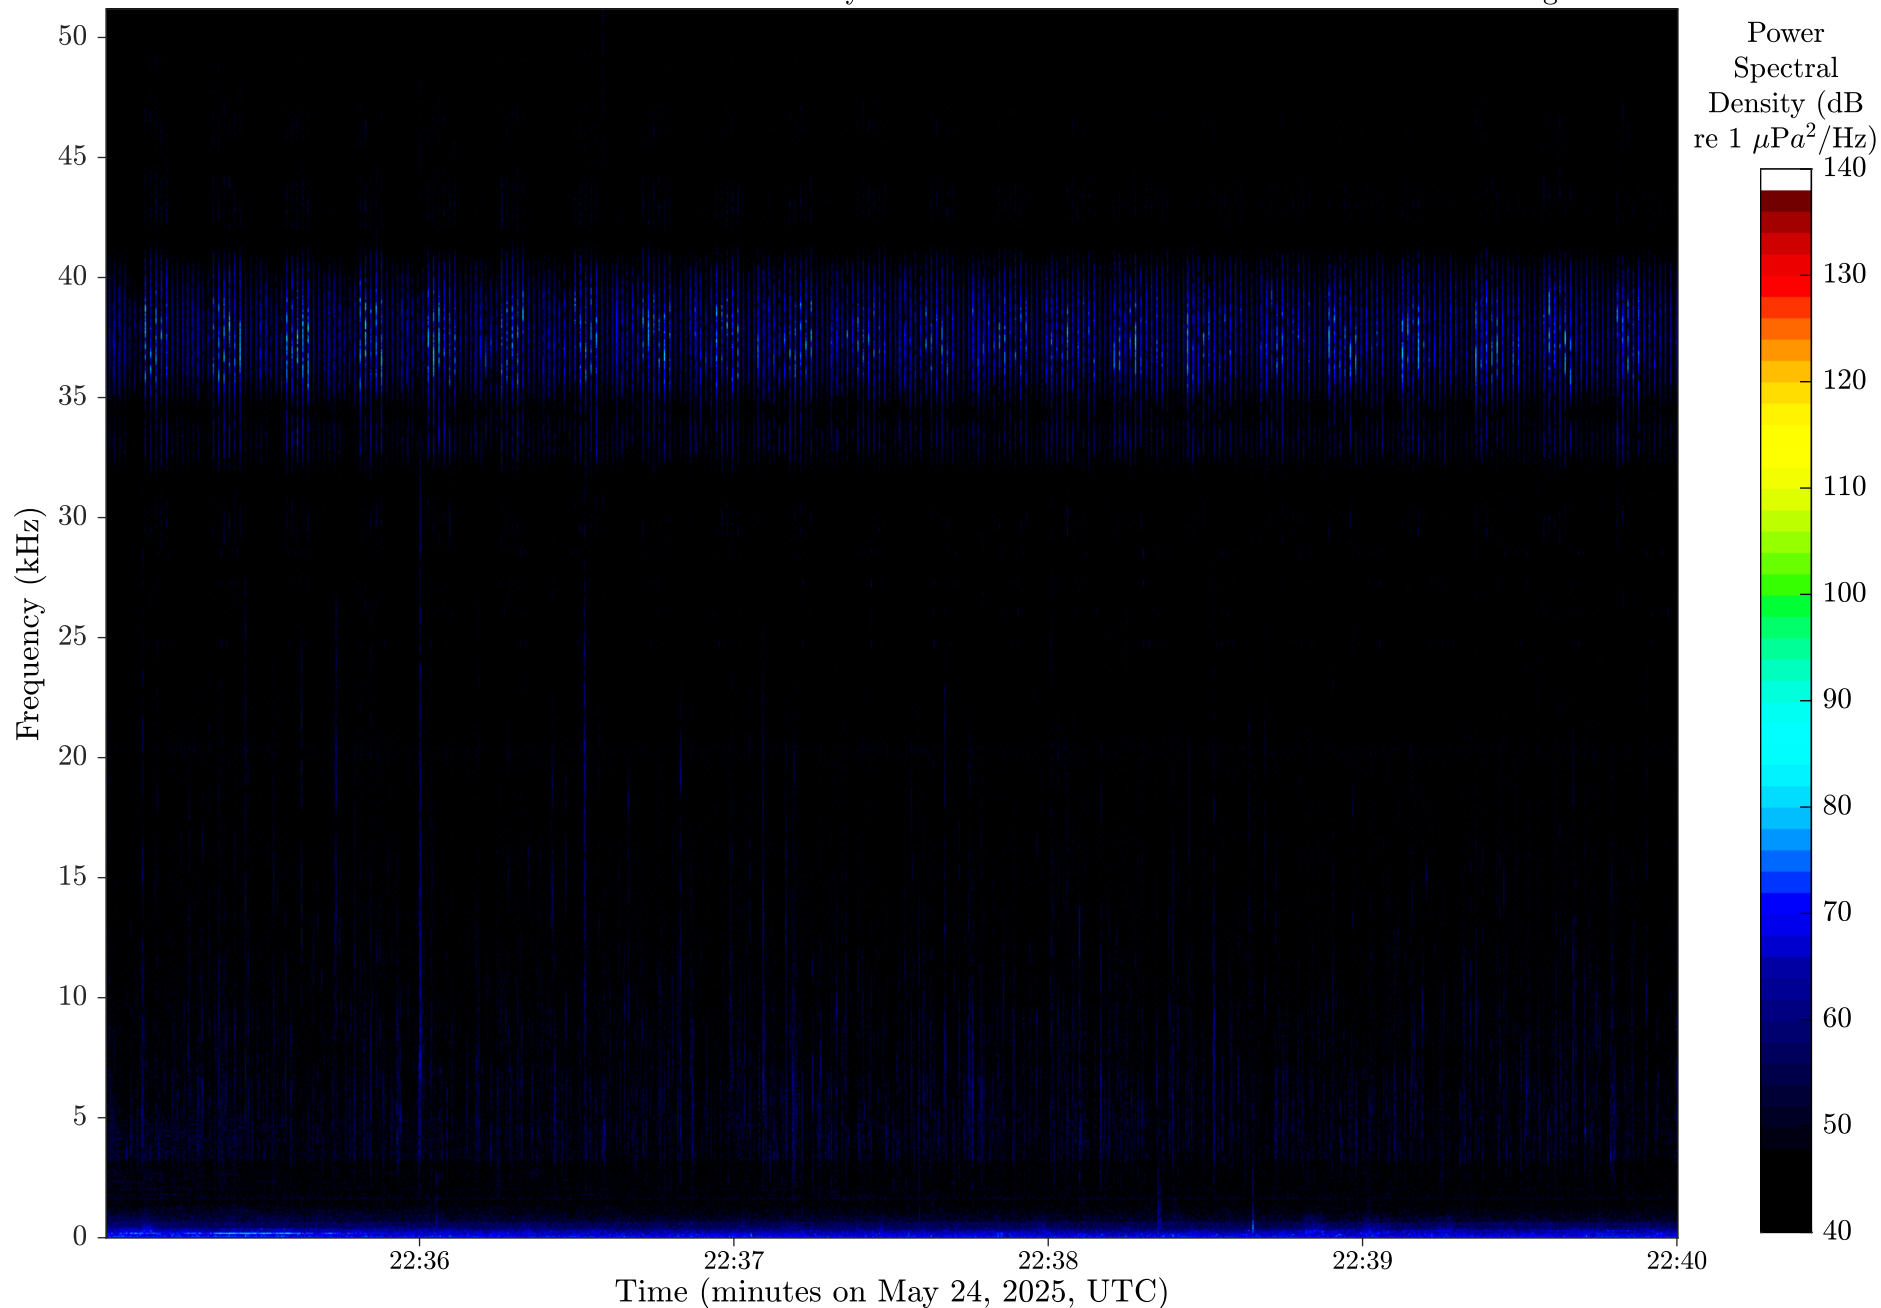

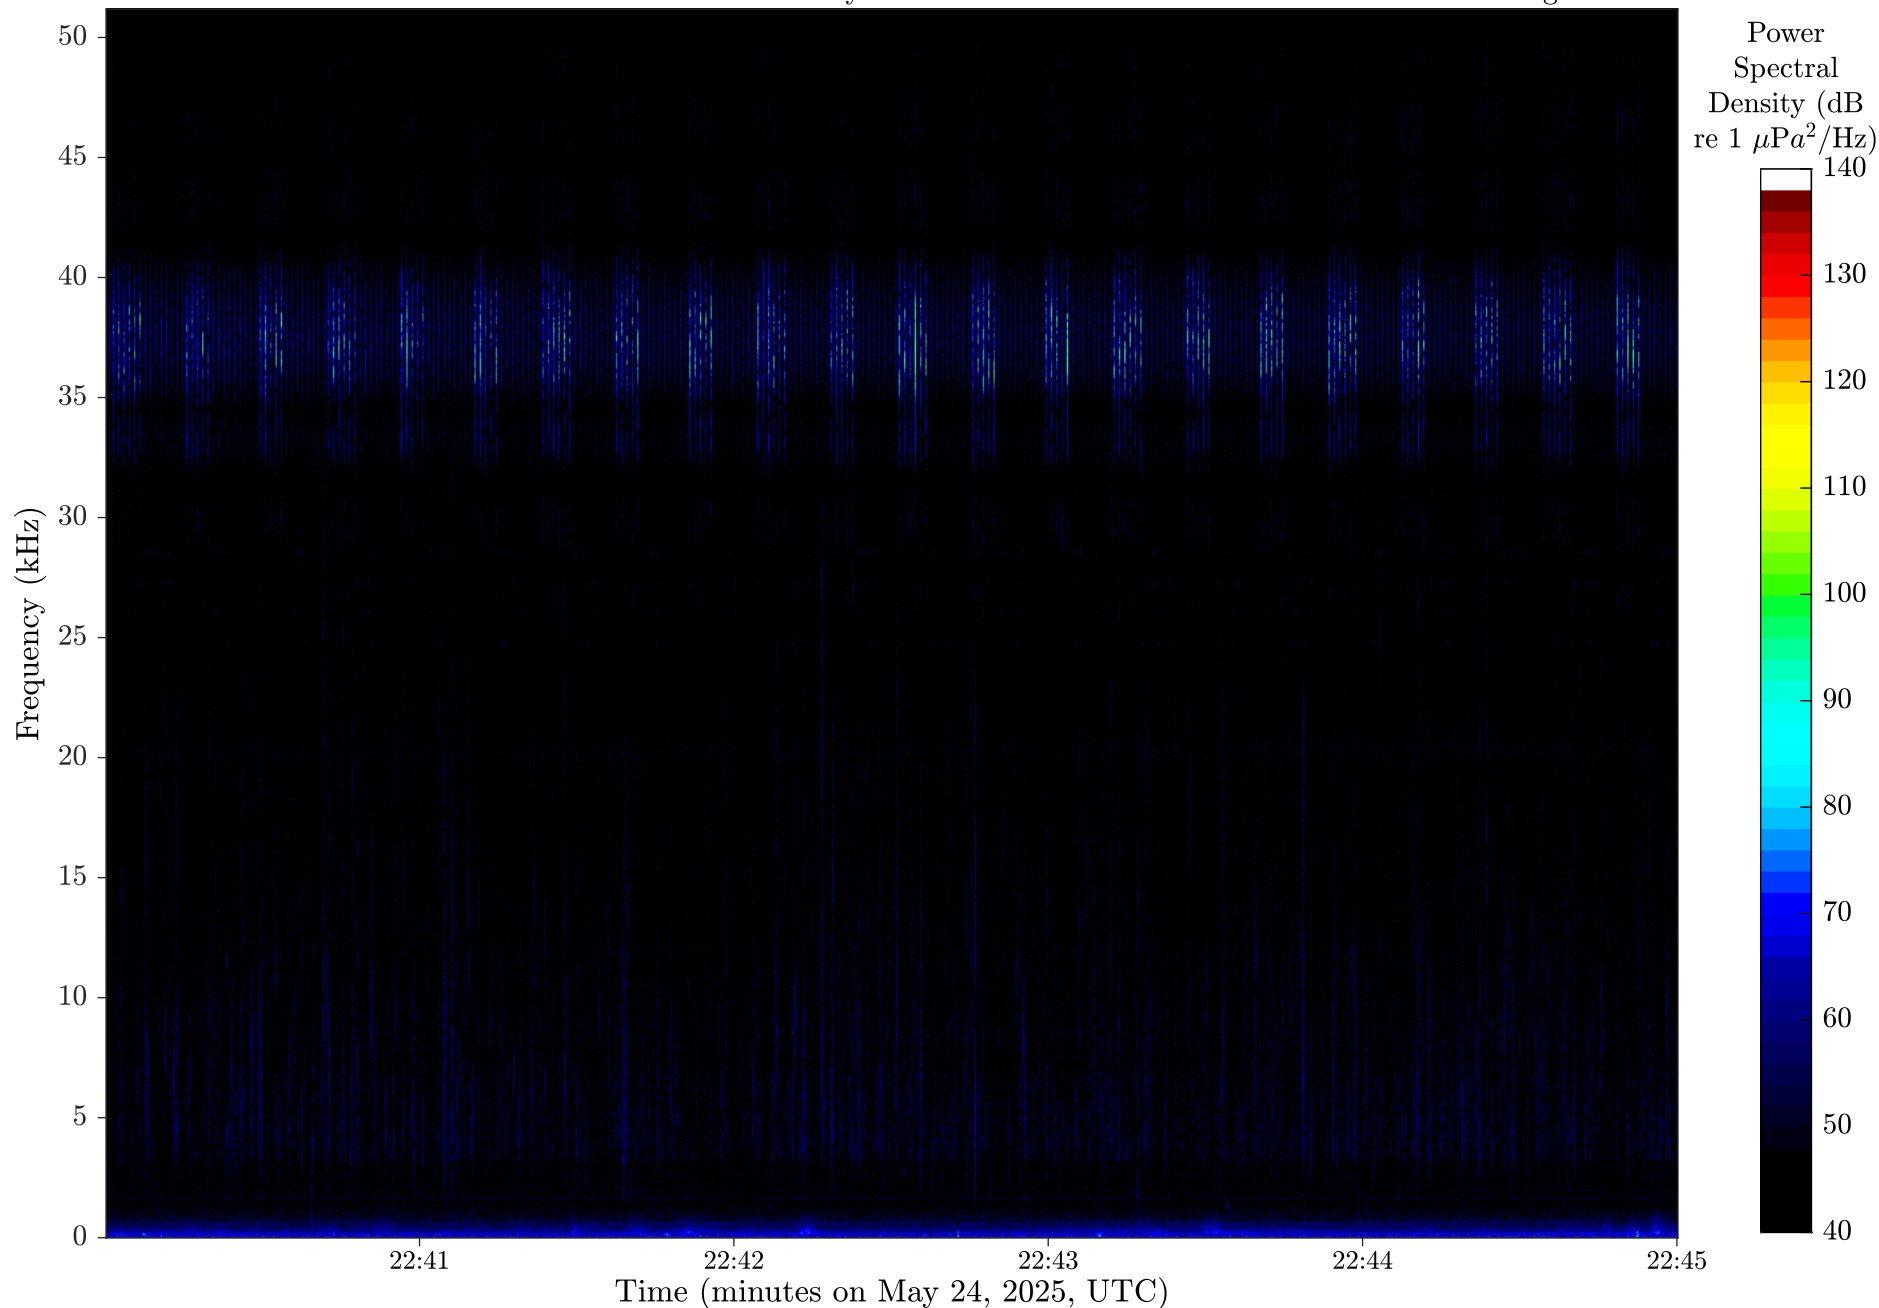


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:52:50 UTC

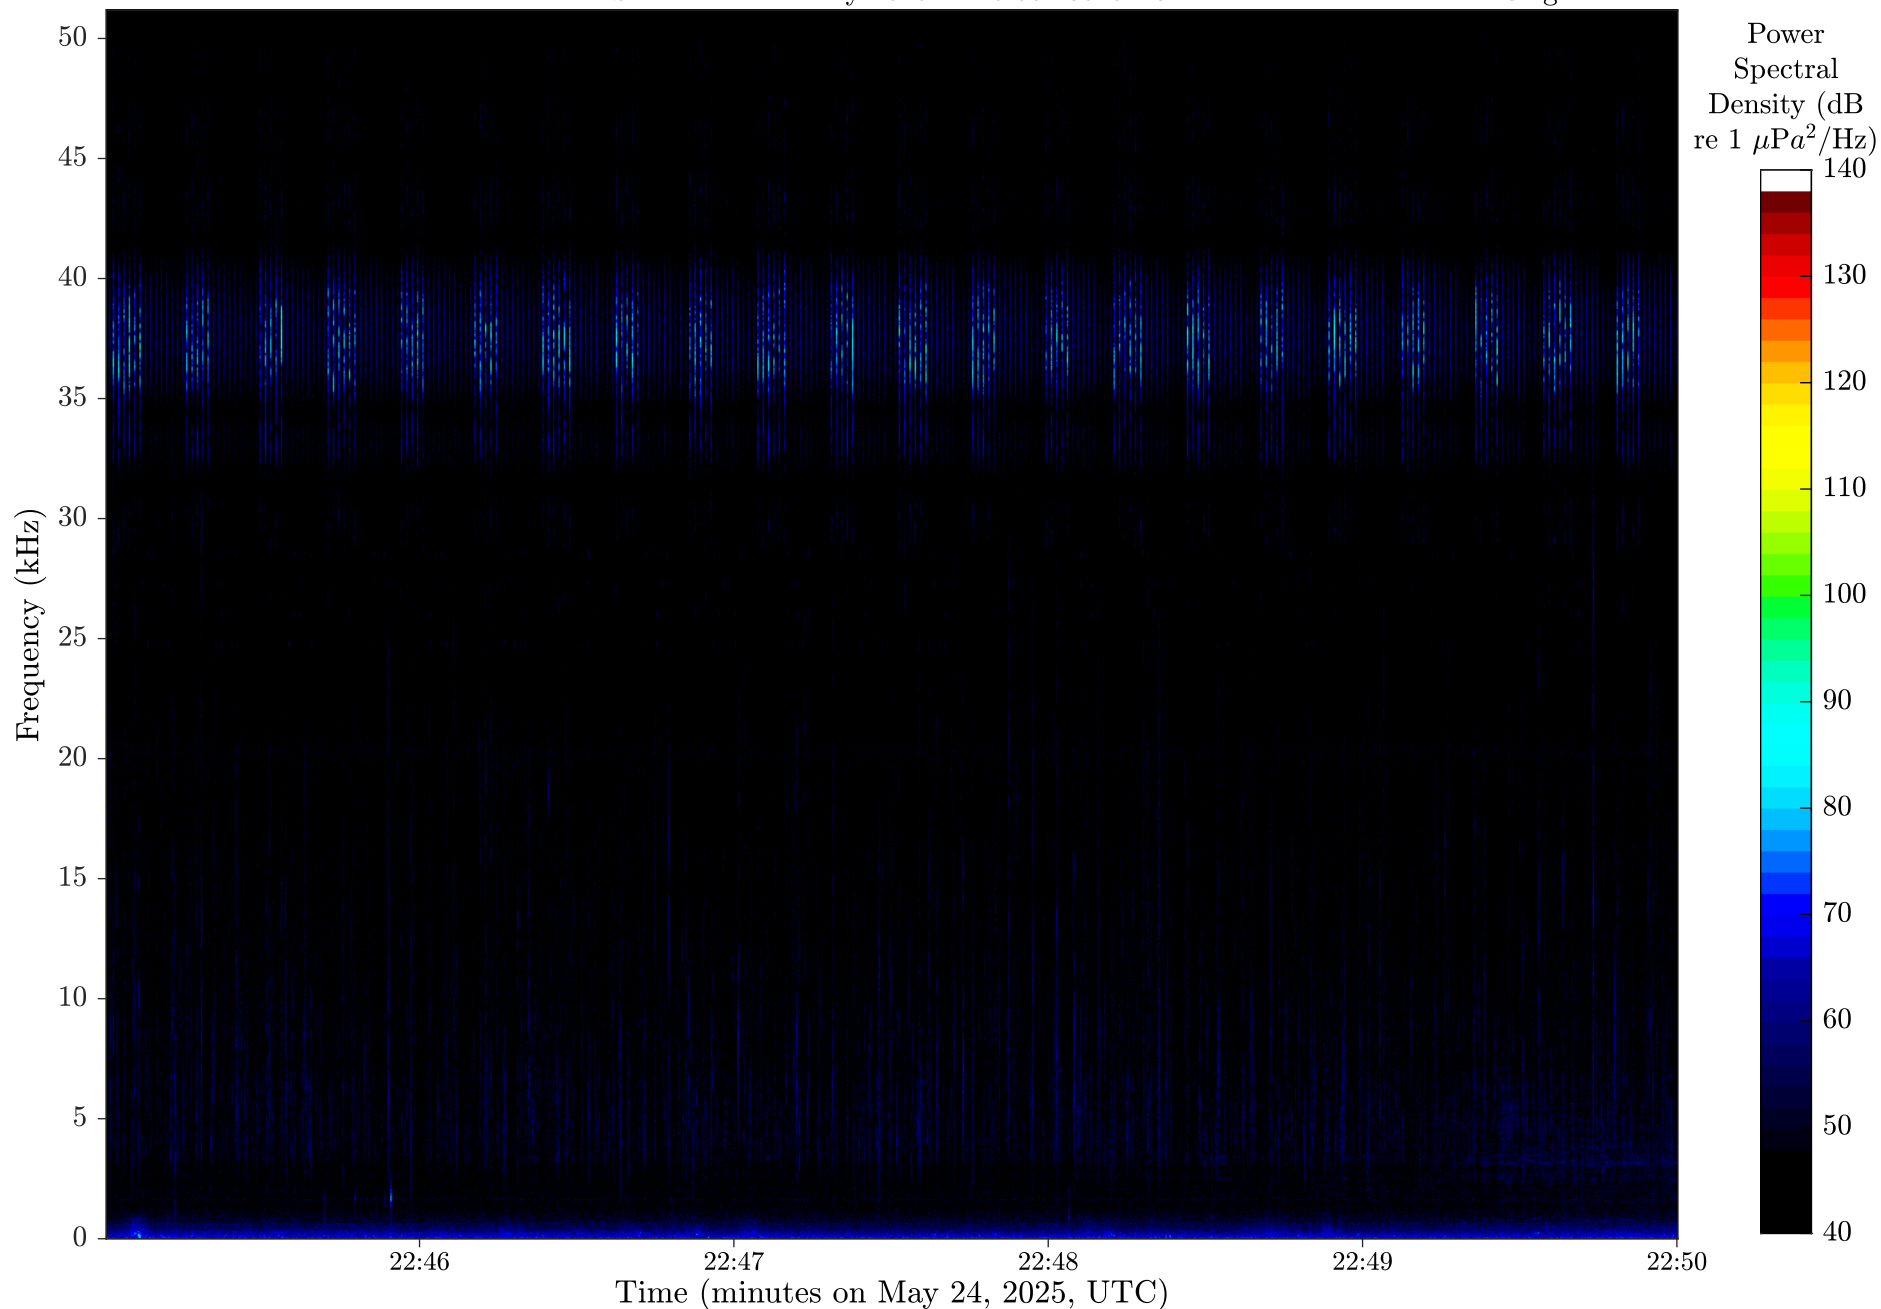


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:53:00 UTC

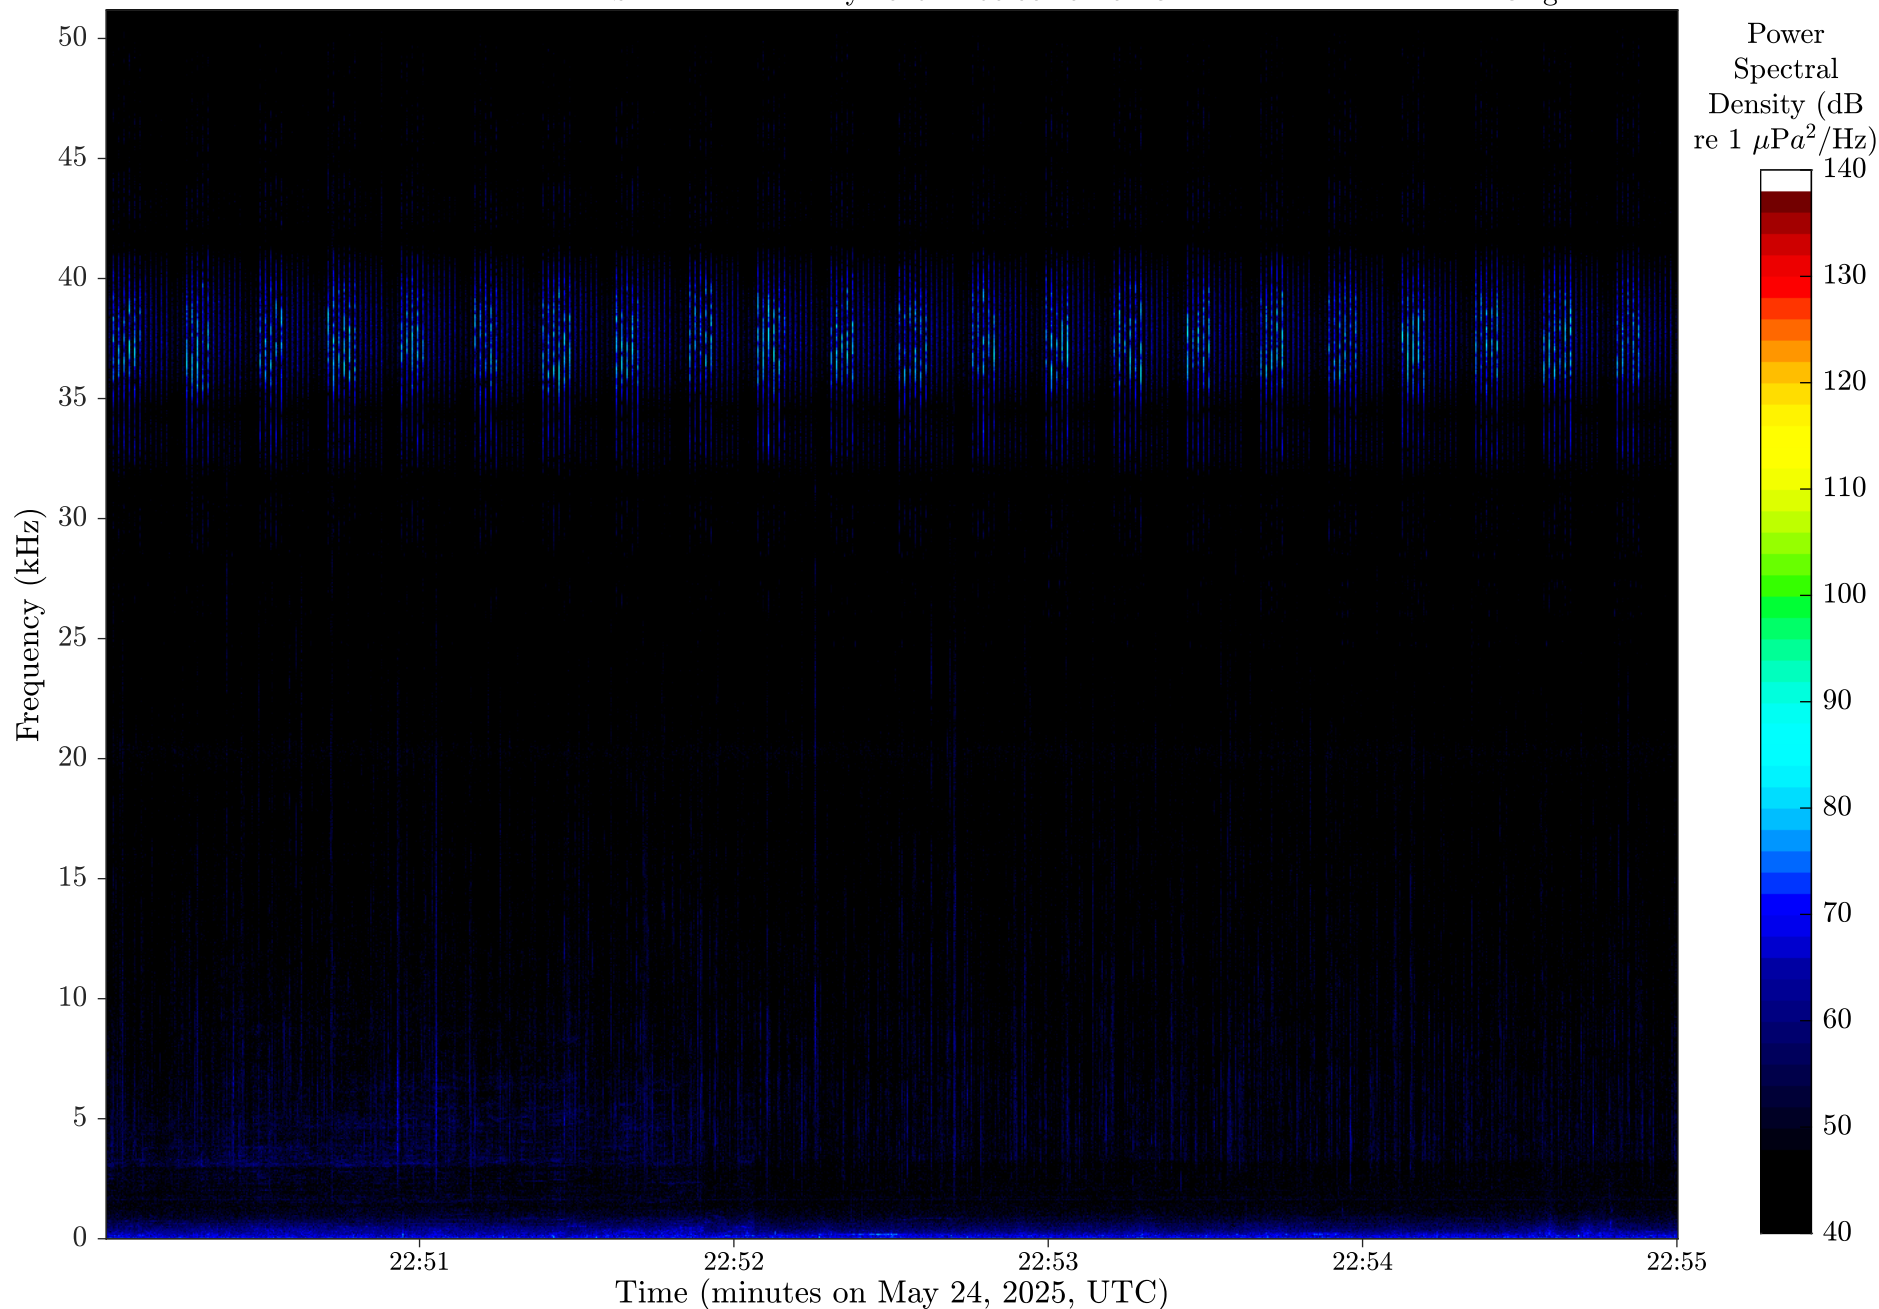


Comments: 34.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:53:08 UTC

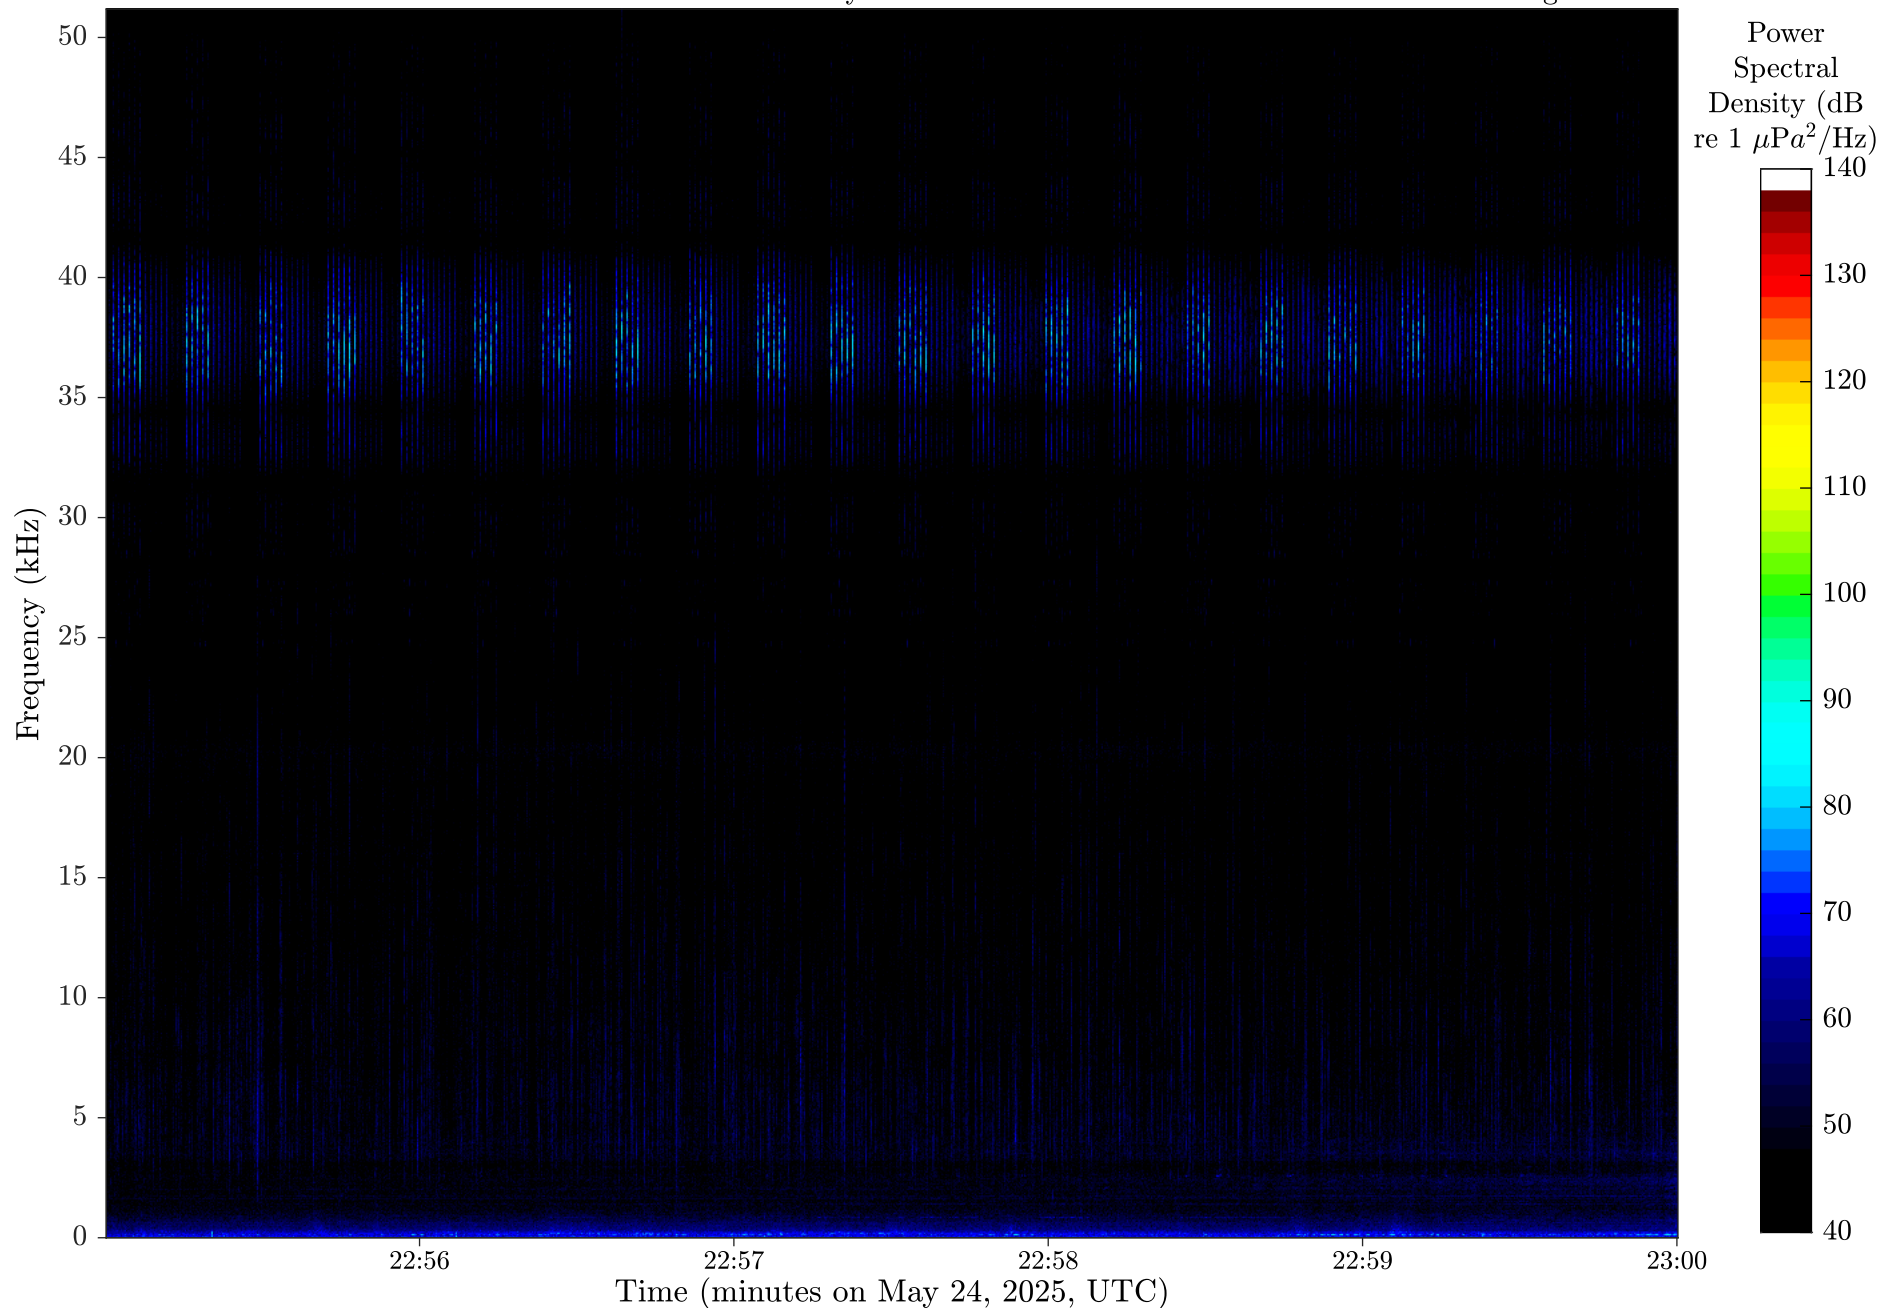

Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:53:17 UTC

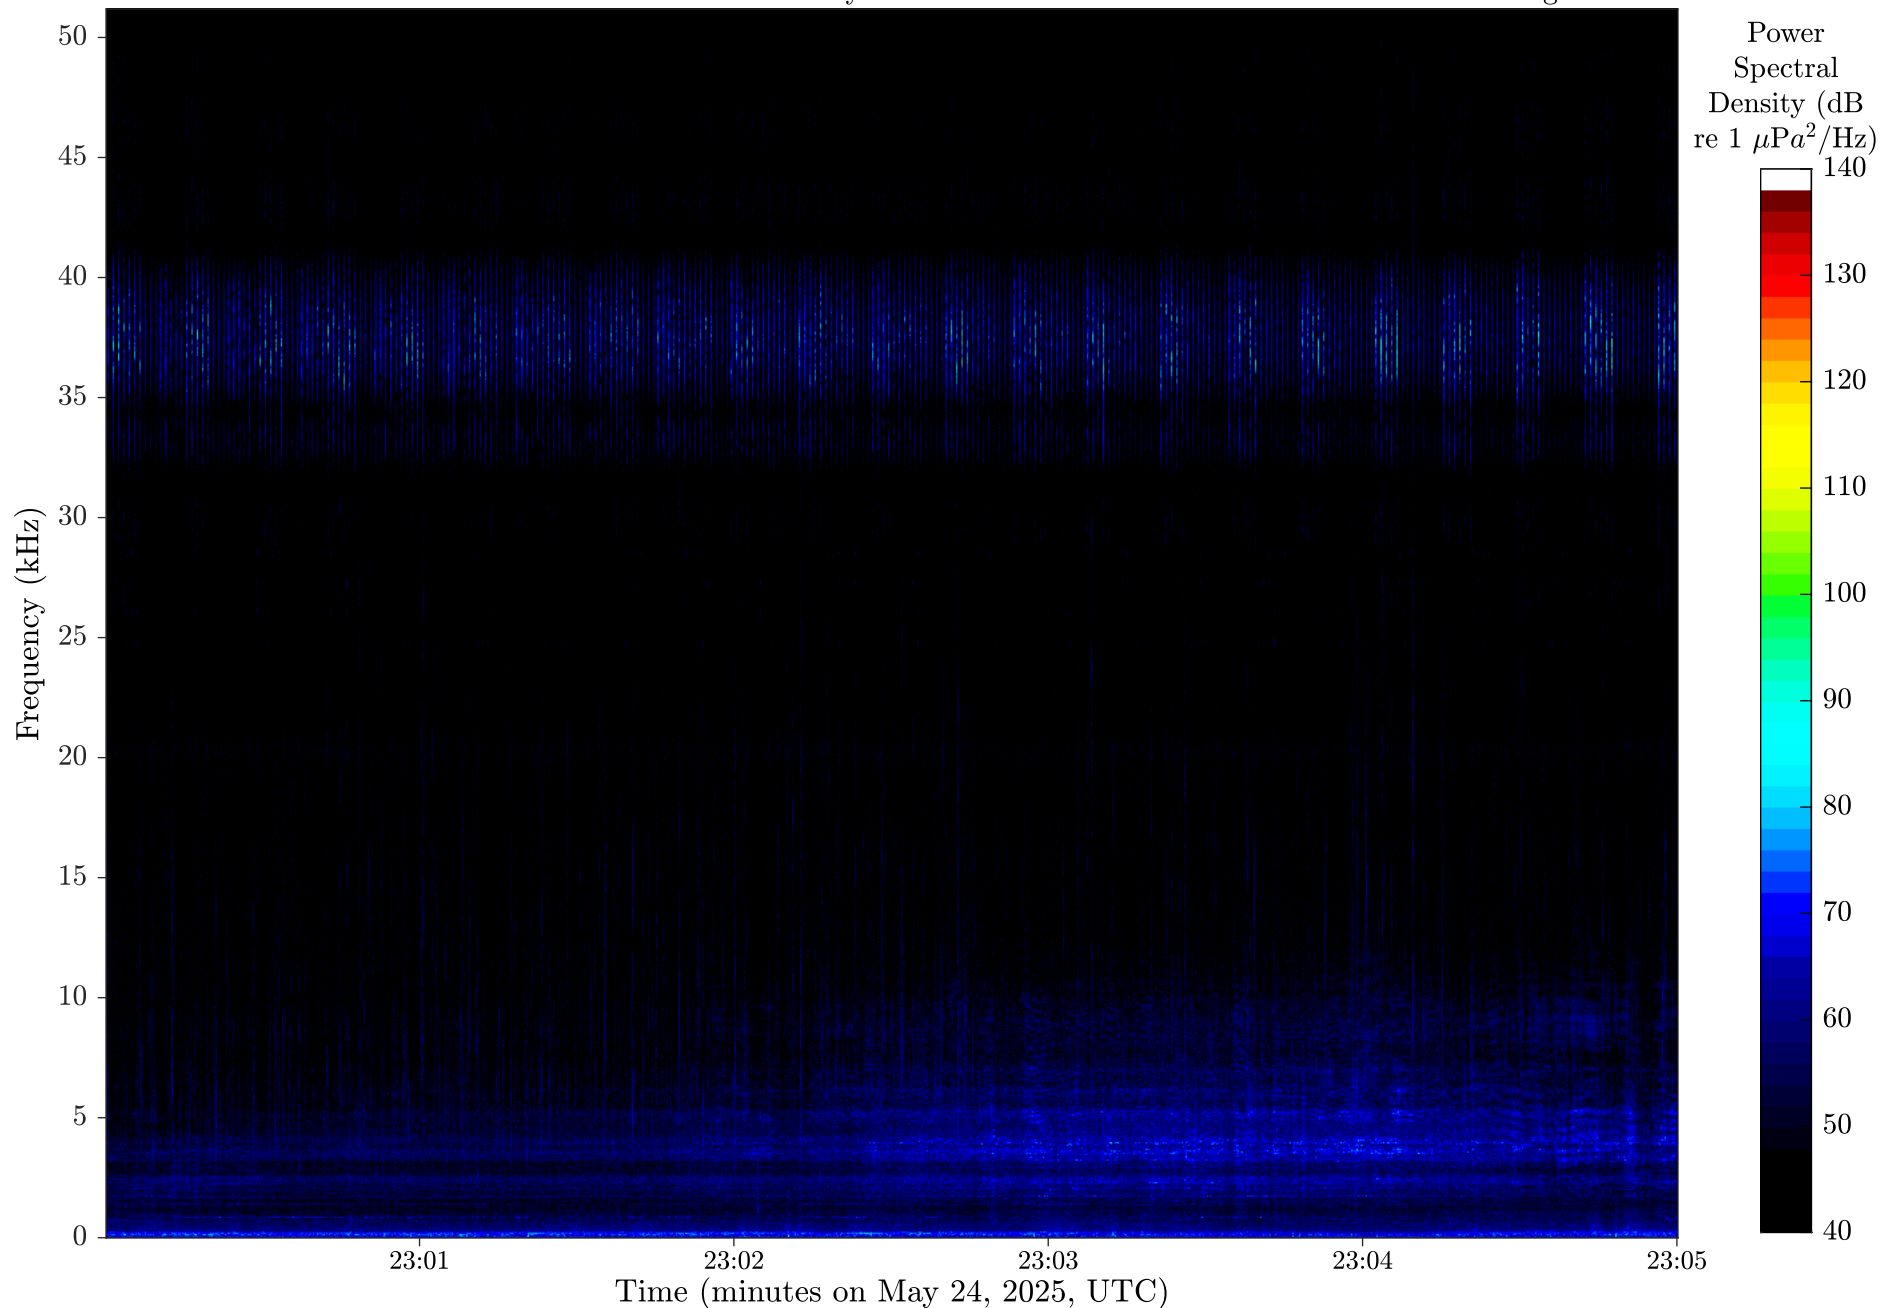

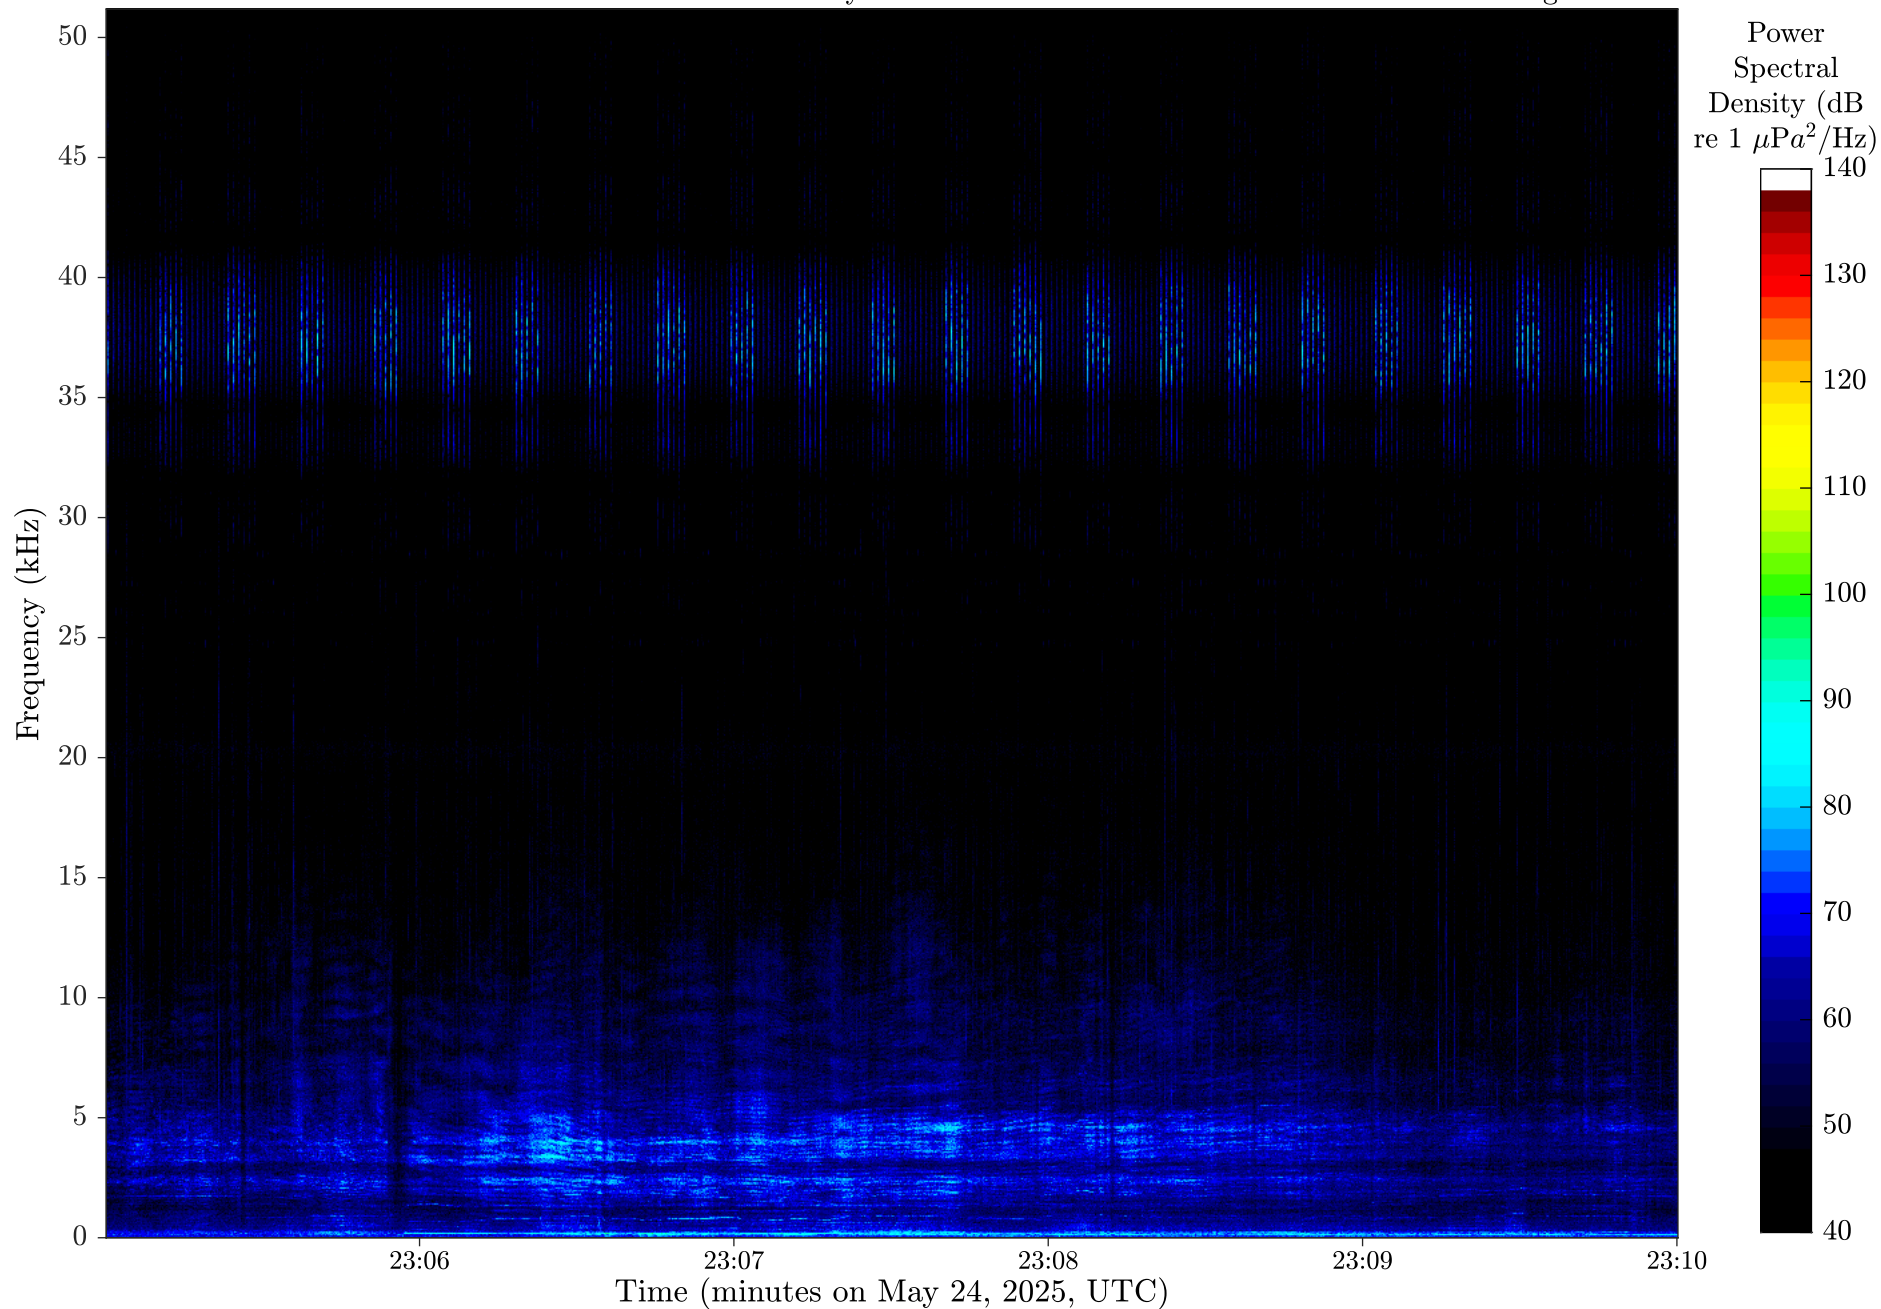


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:53:34 UTC

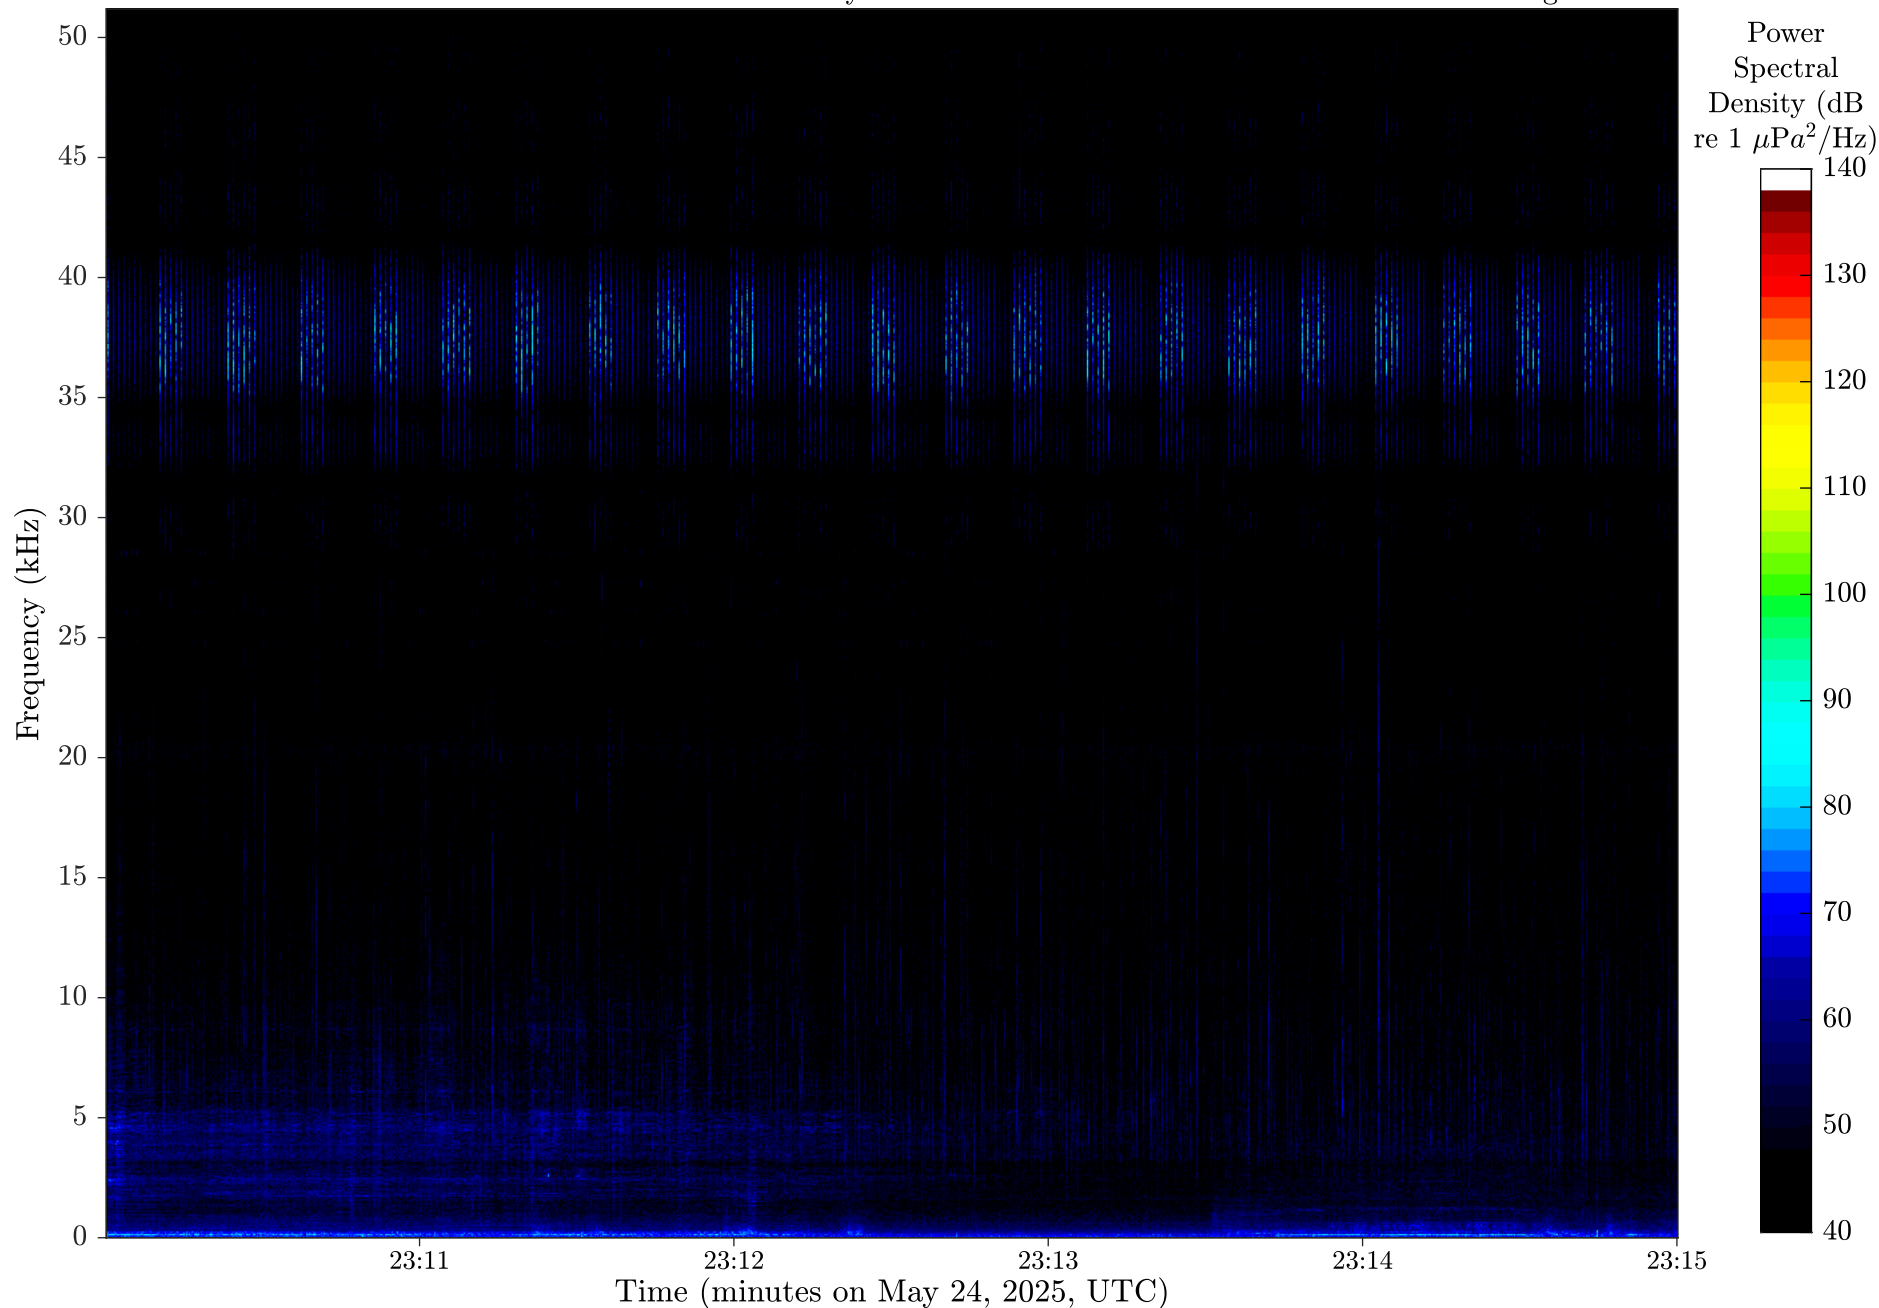


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:53:42 UTC

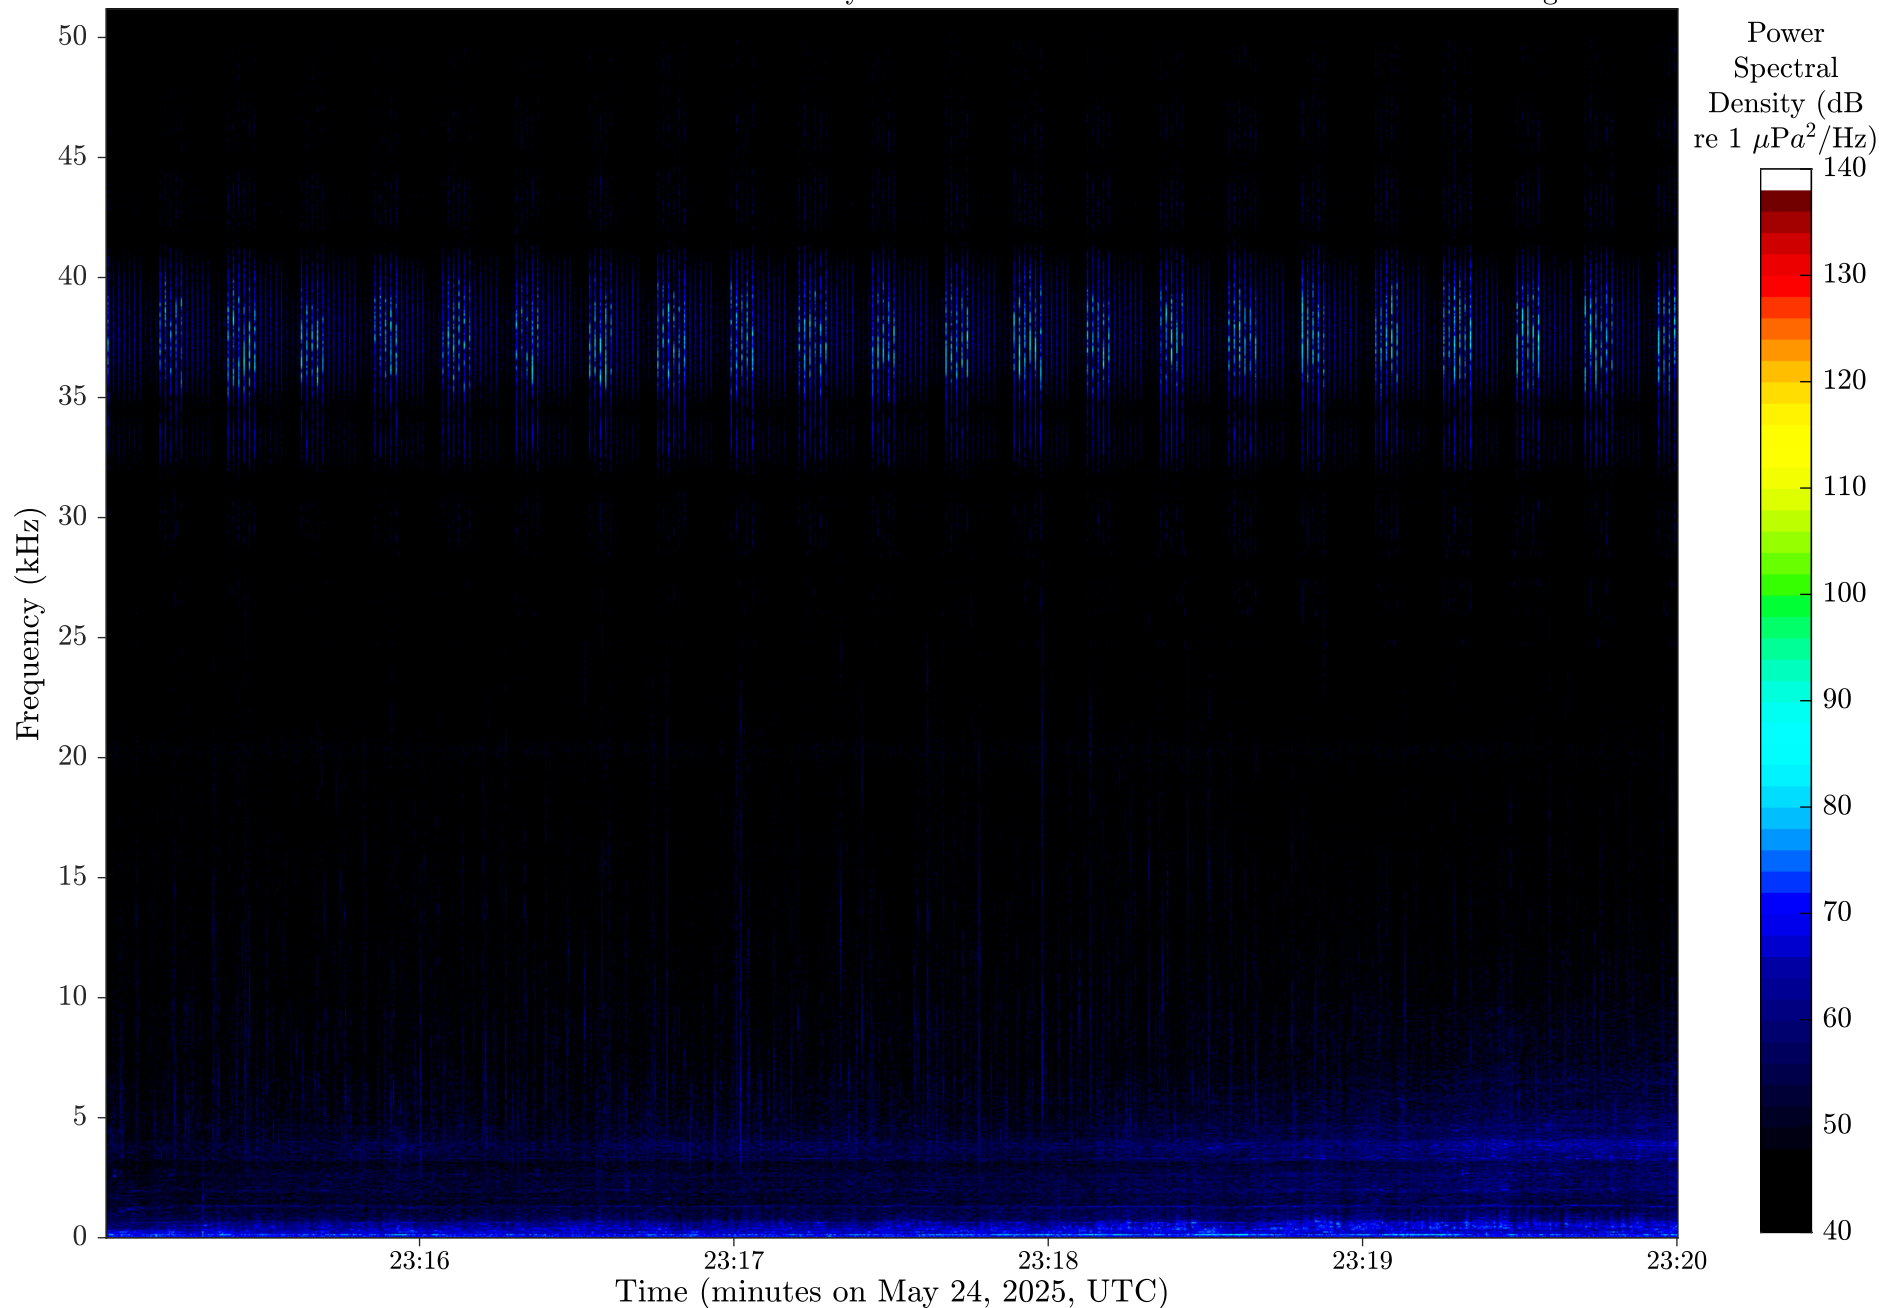


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:53:50 UTC

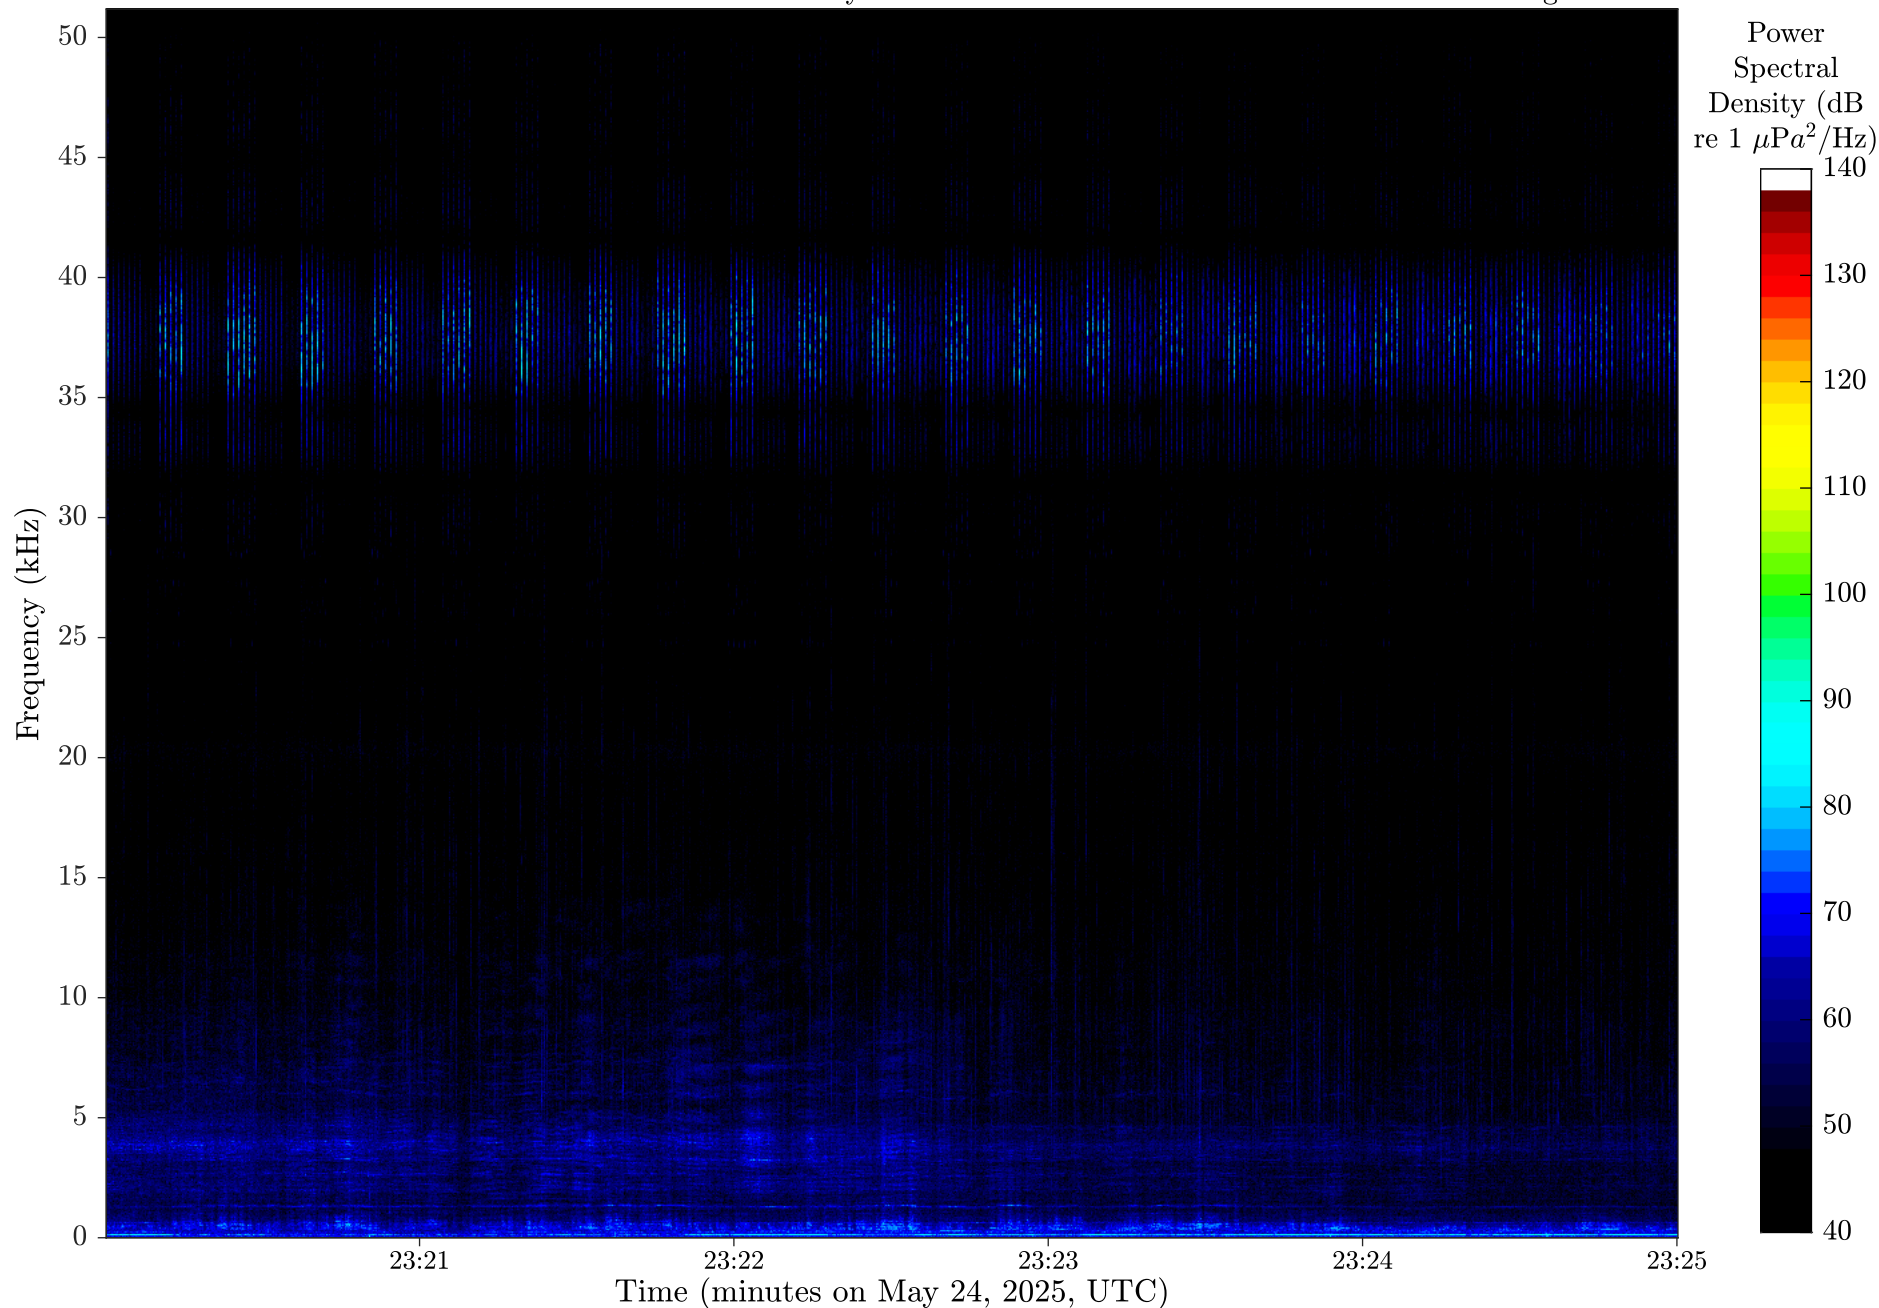


Comments: 30.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:53:58 UTC

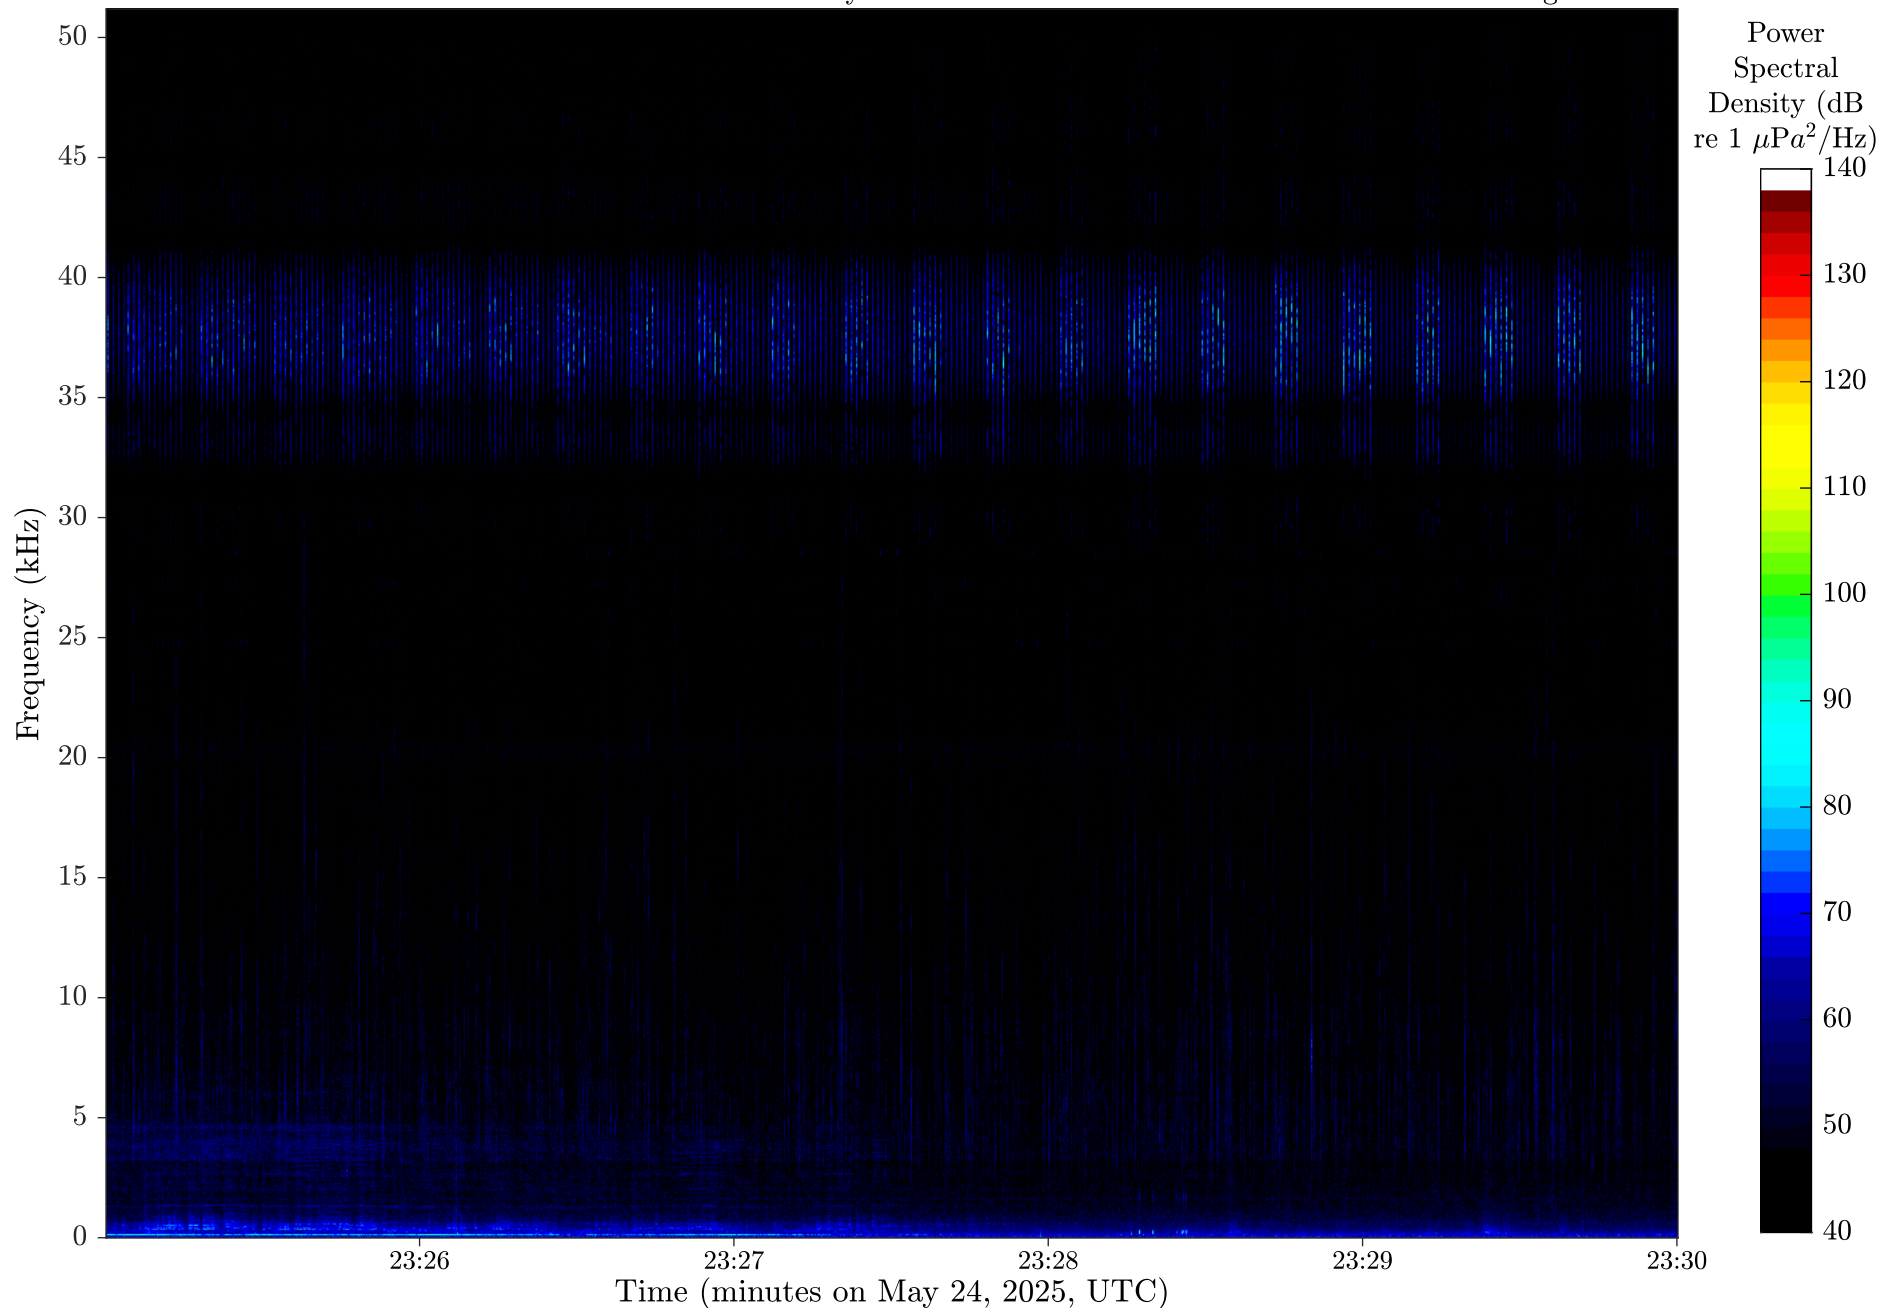


Comments: 31.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:54:07 UTC

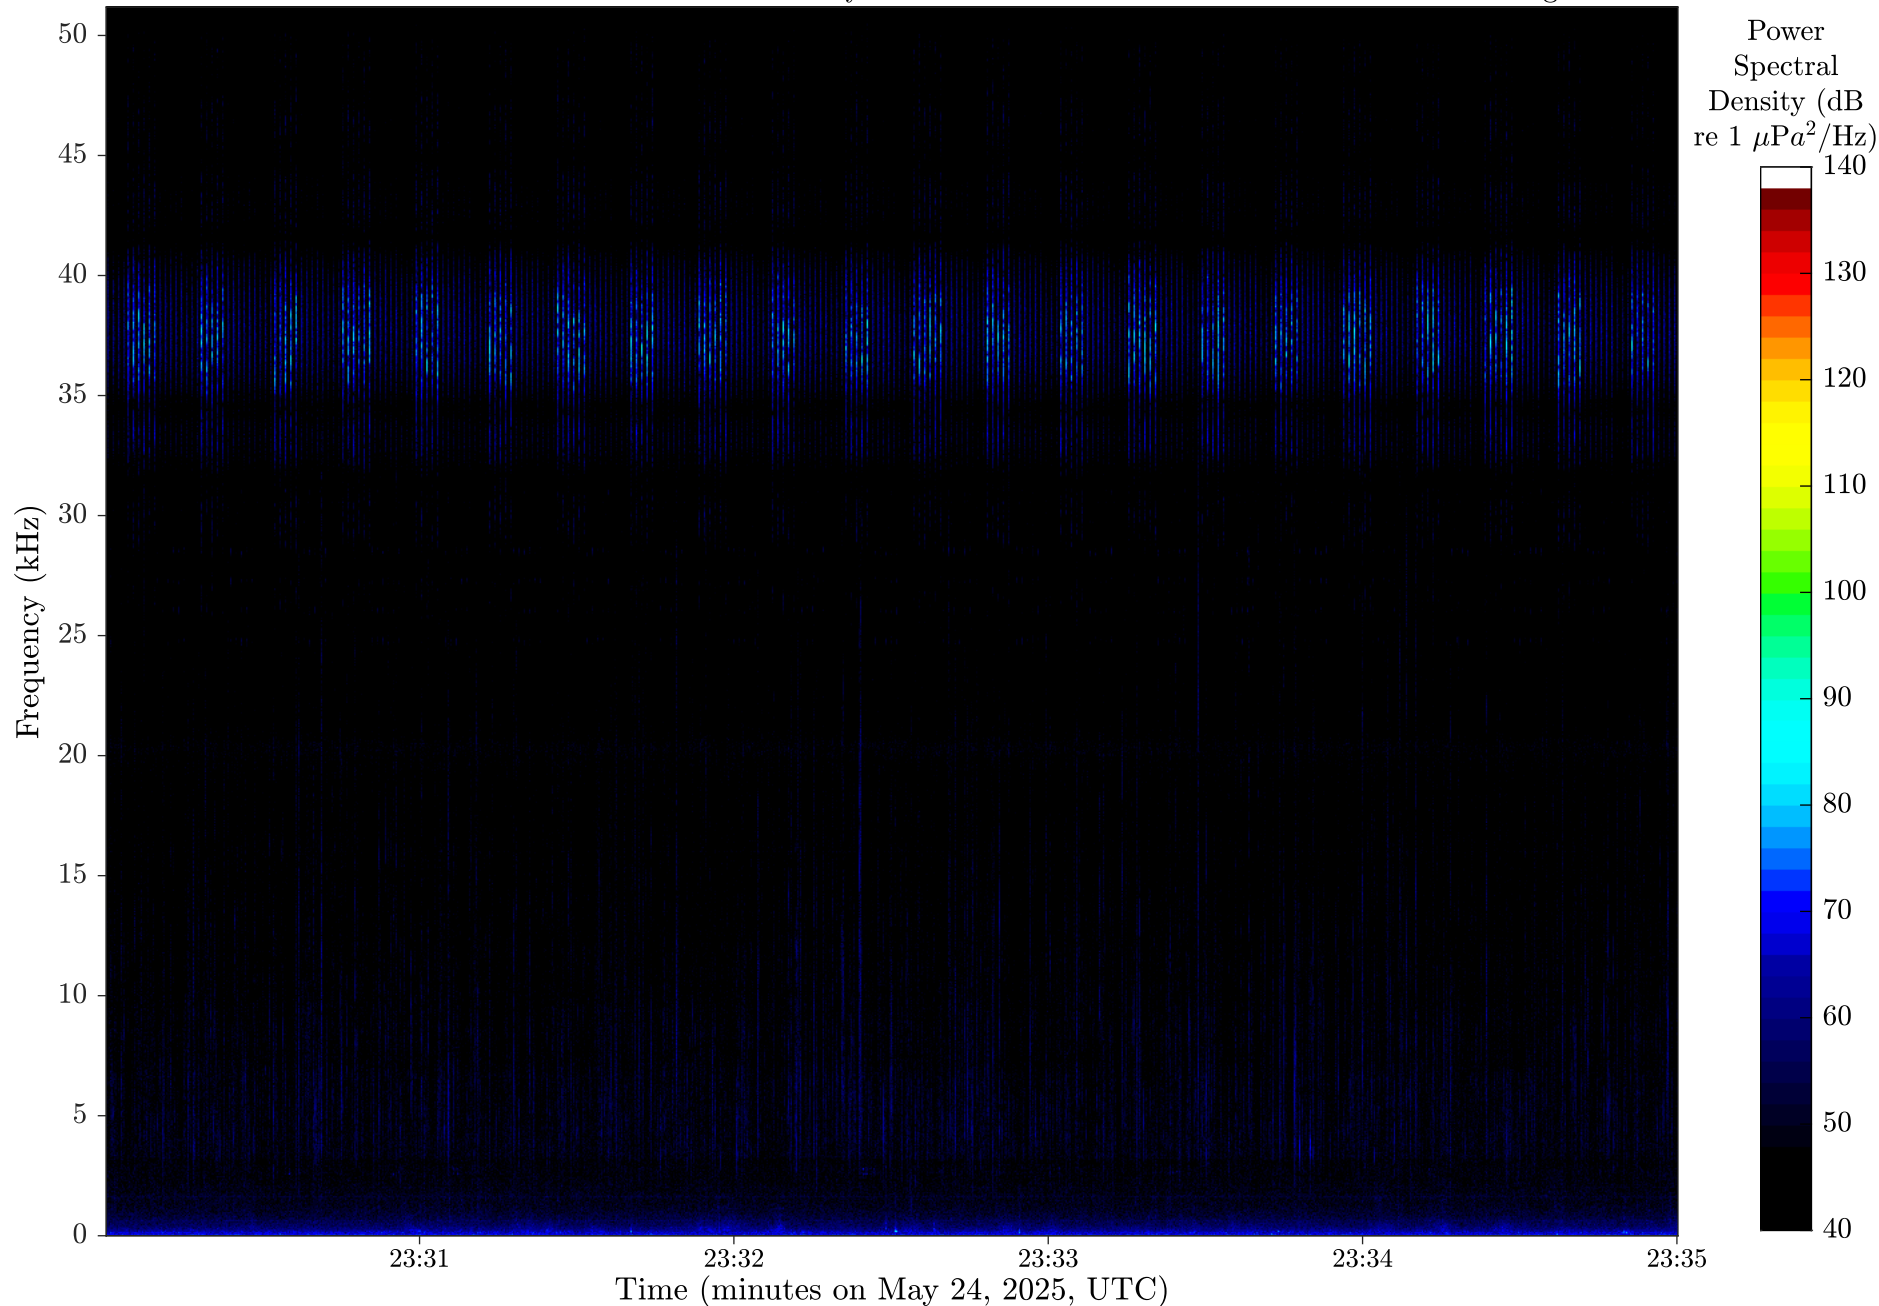

Comments: 33.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:54:16 UTC

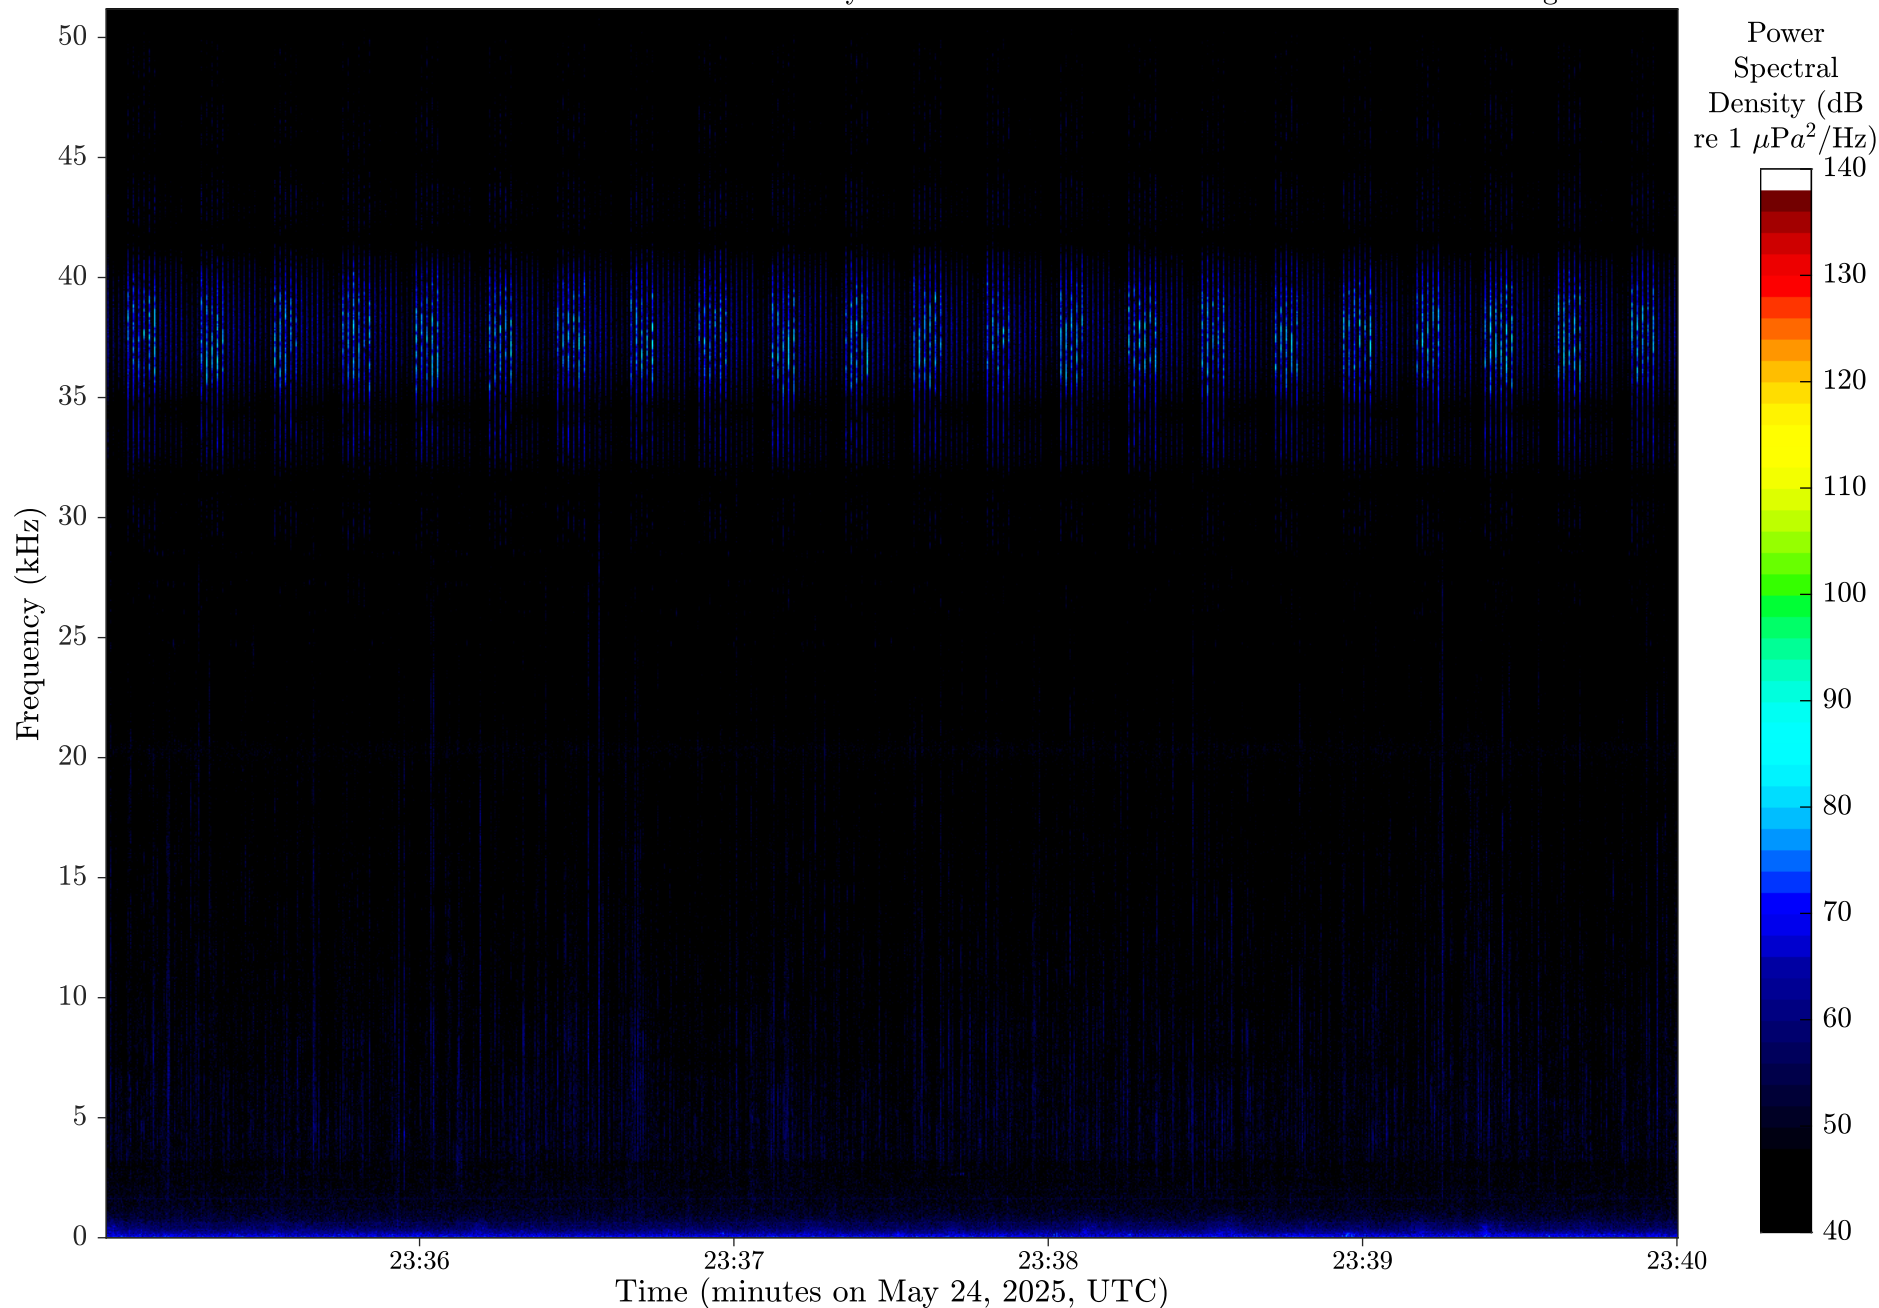

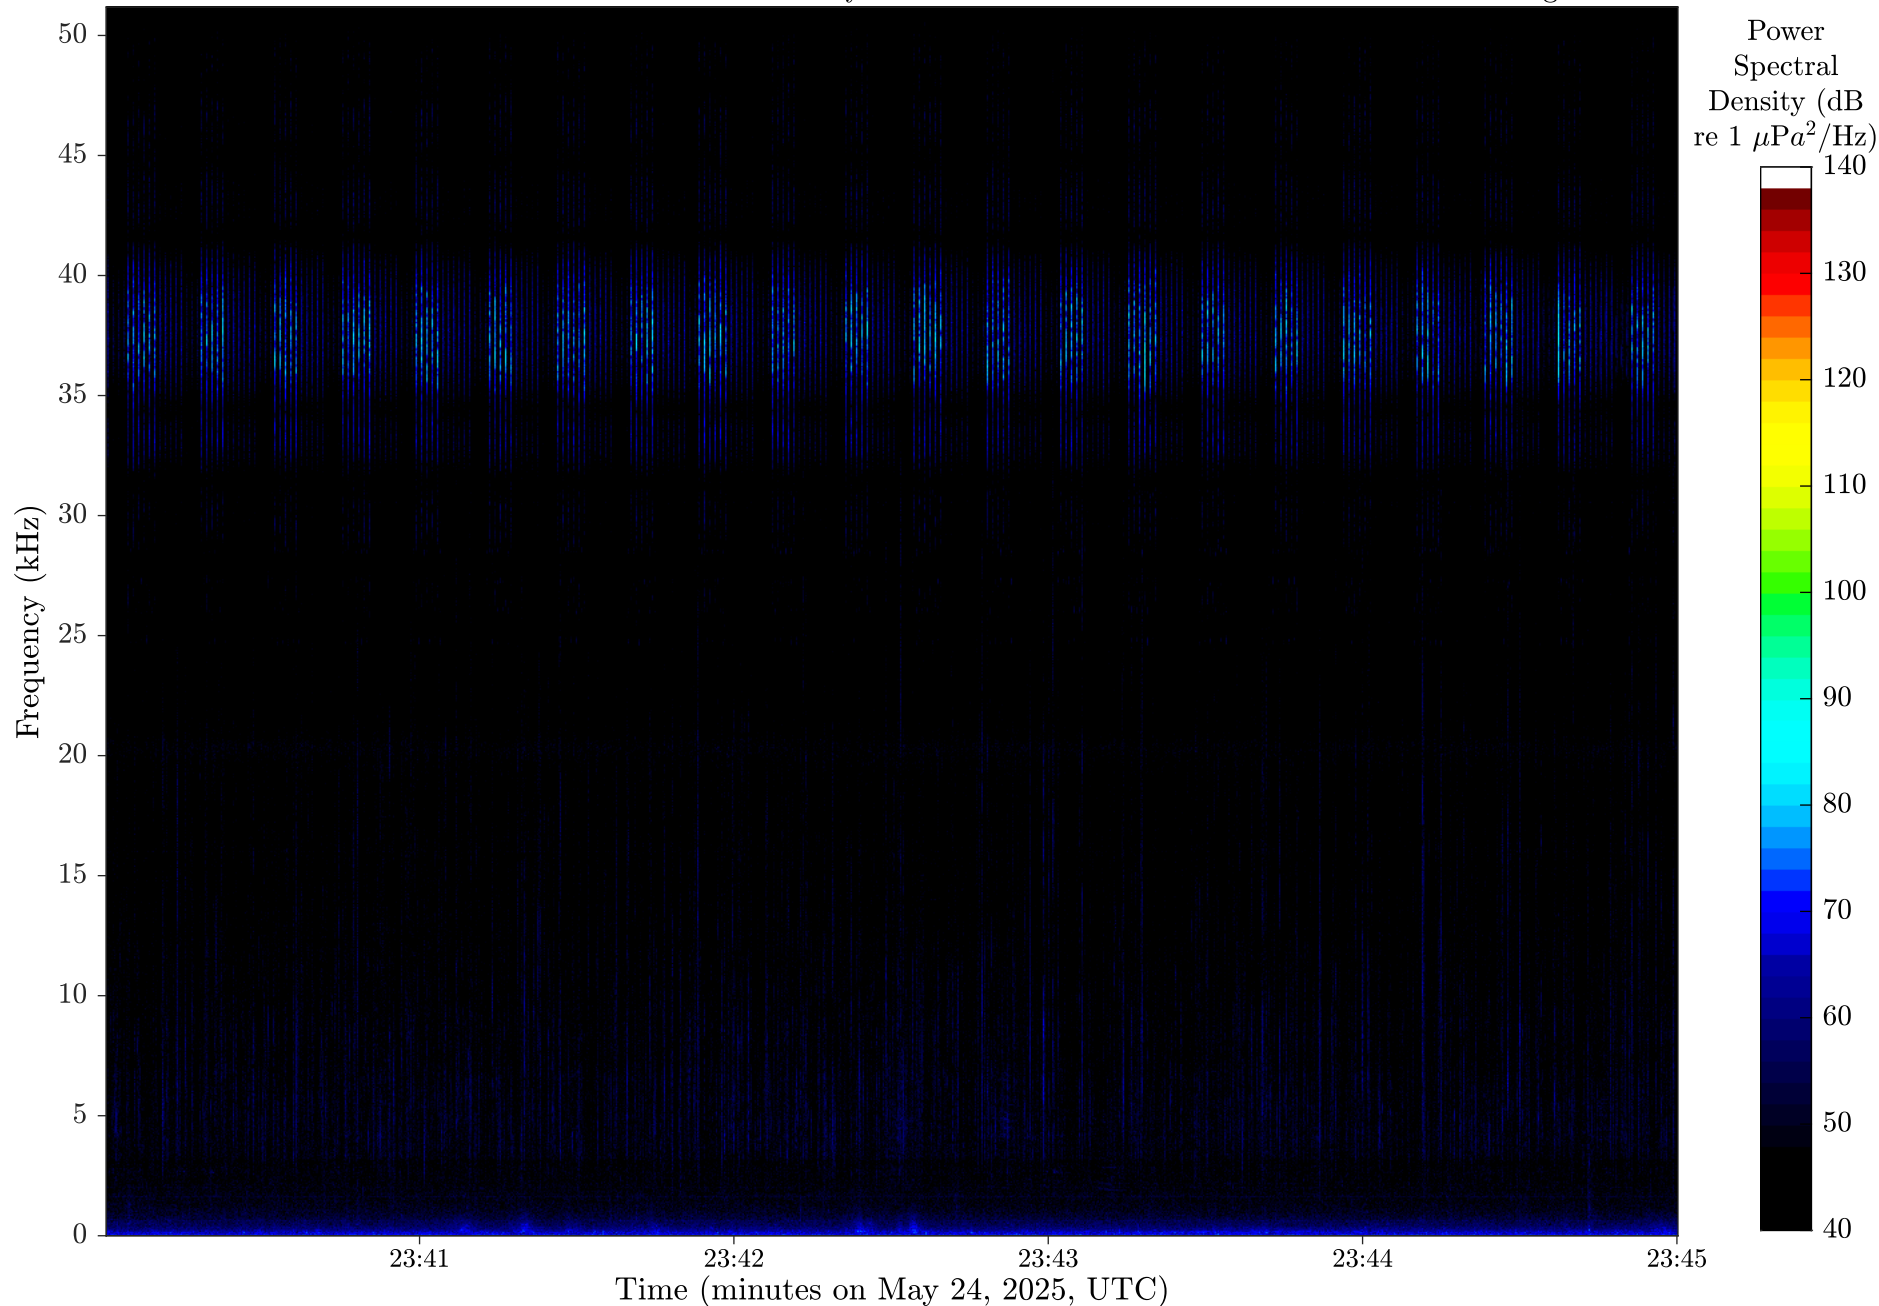


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:54:33 UTC

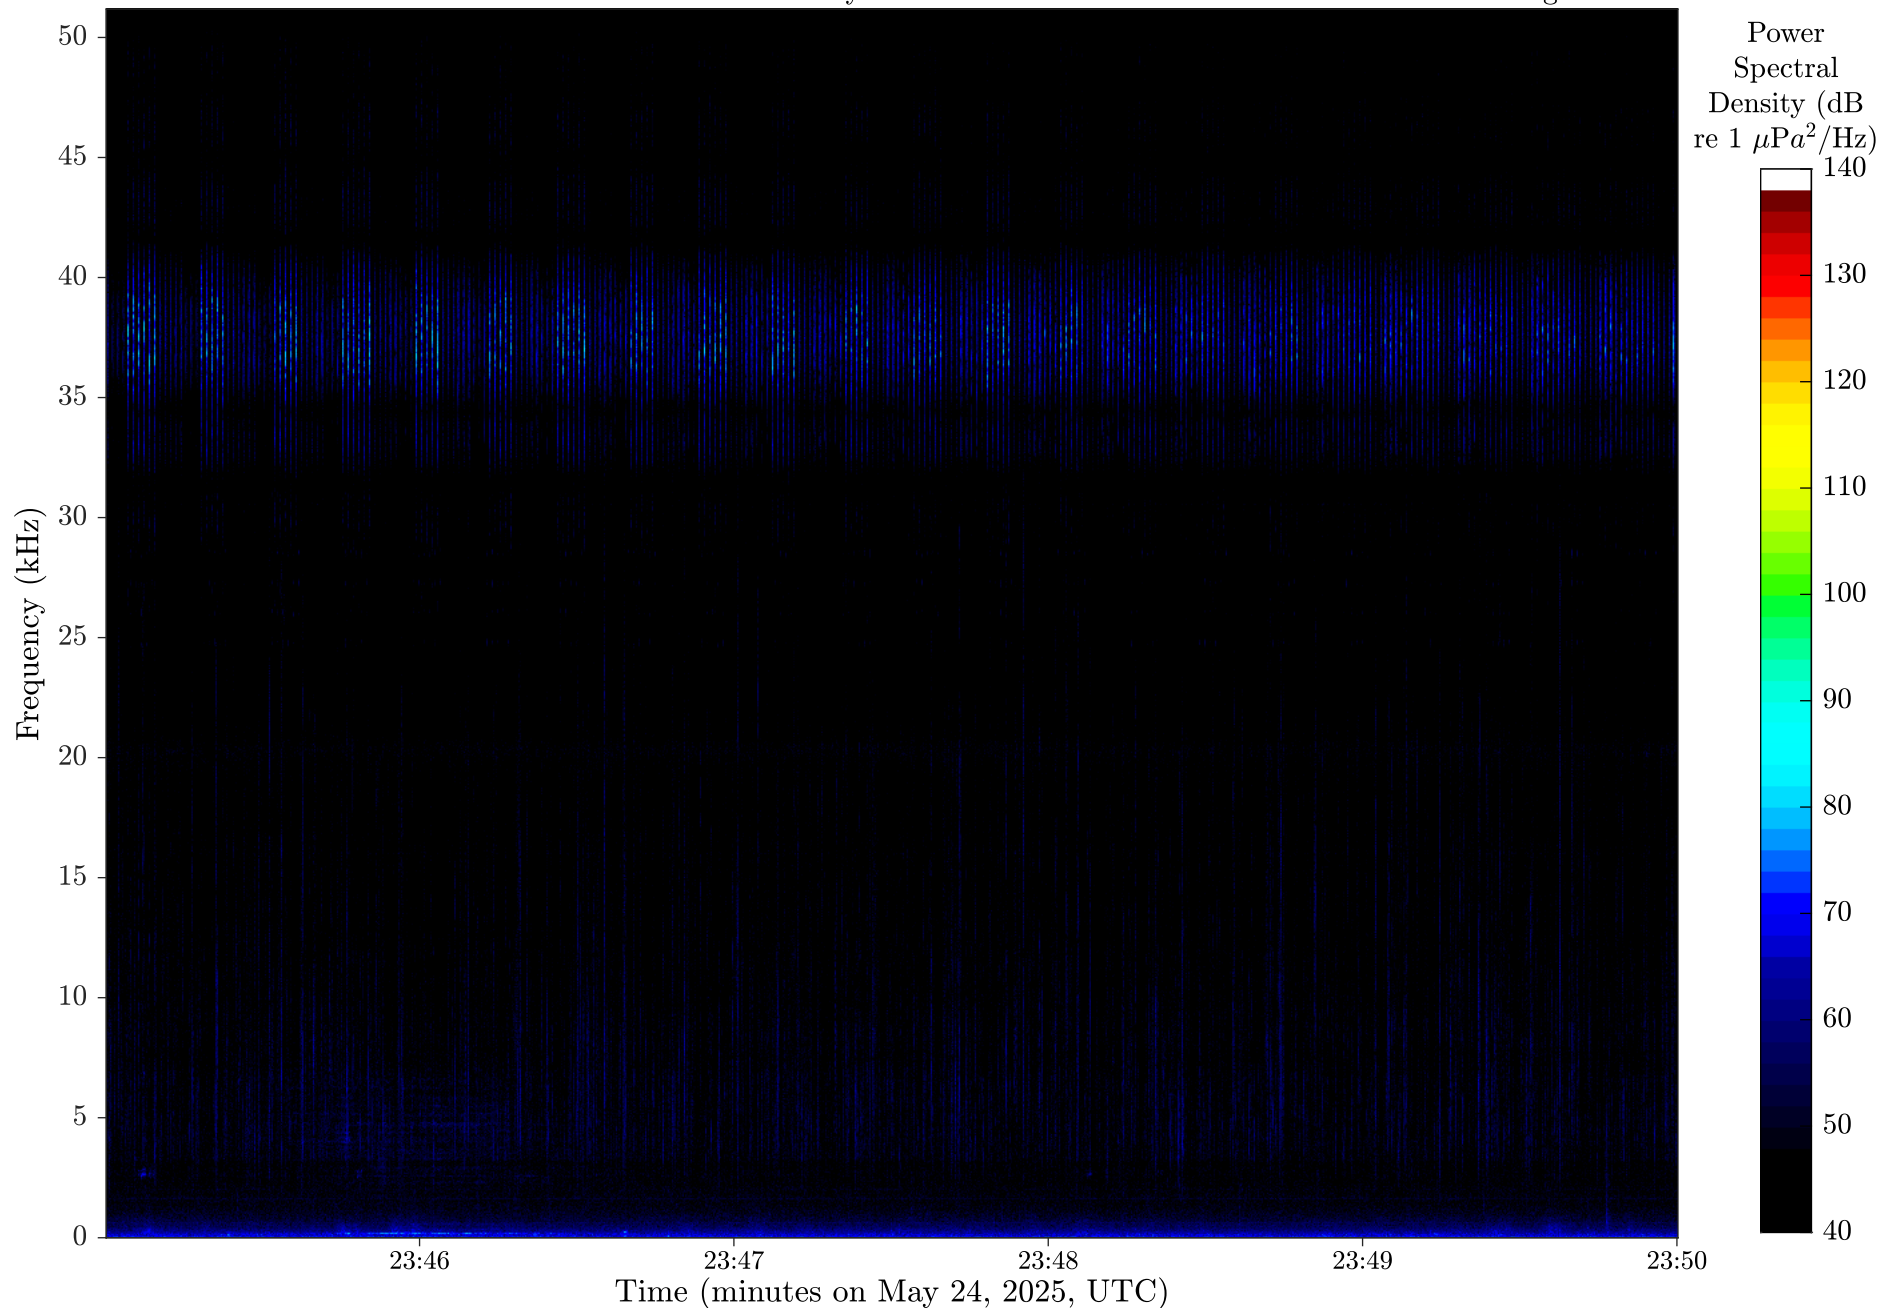

Comments: 34.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:54:41 UTC

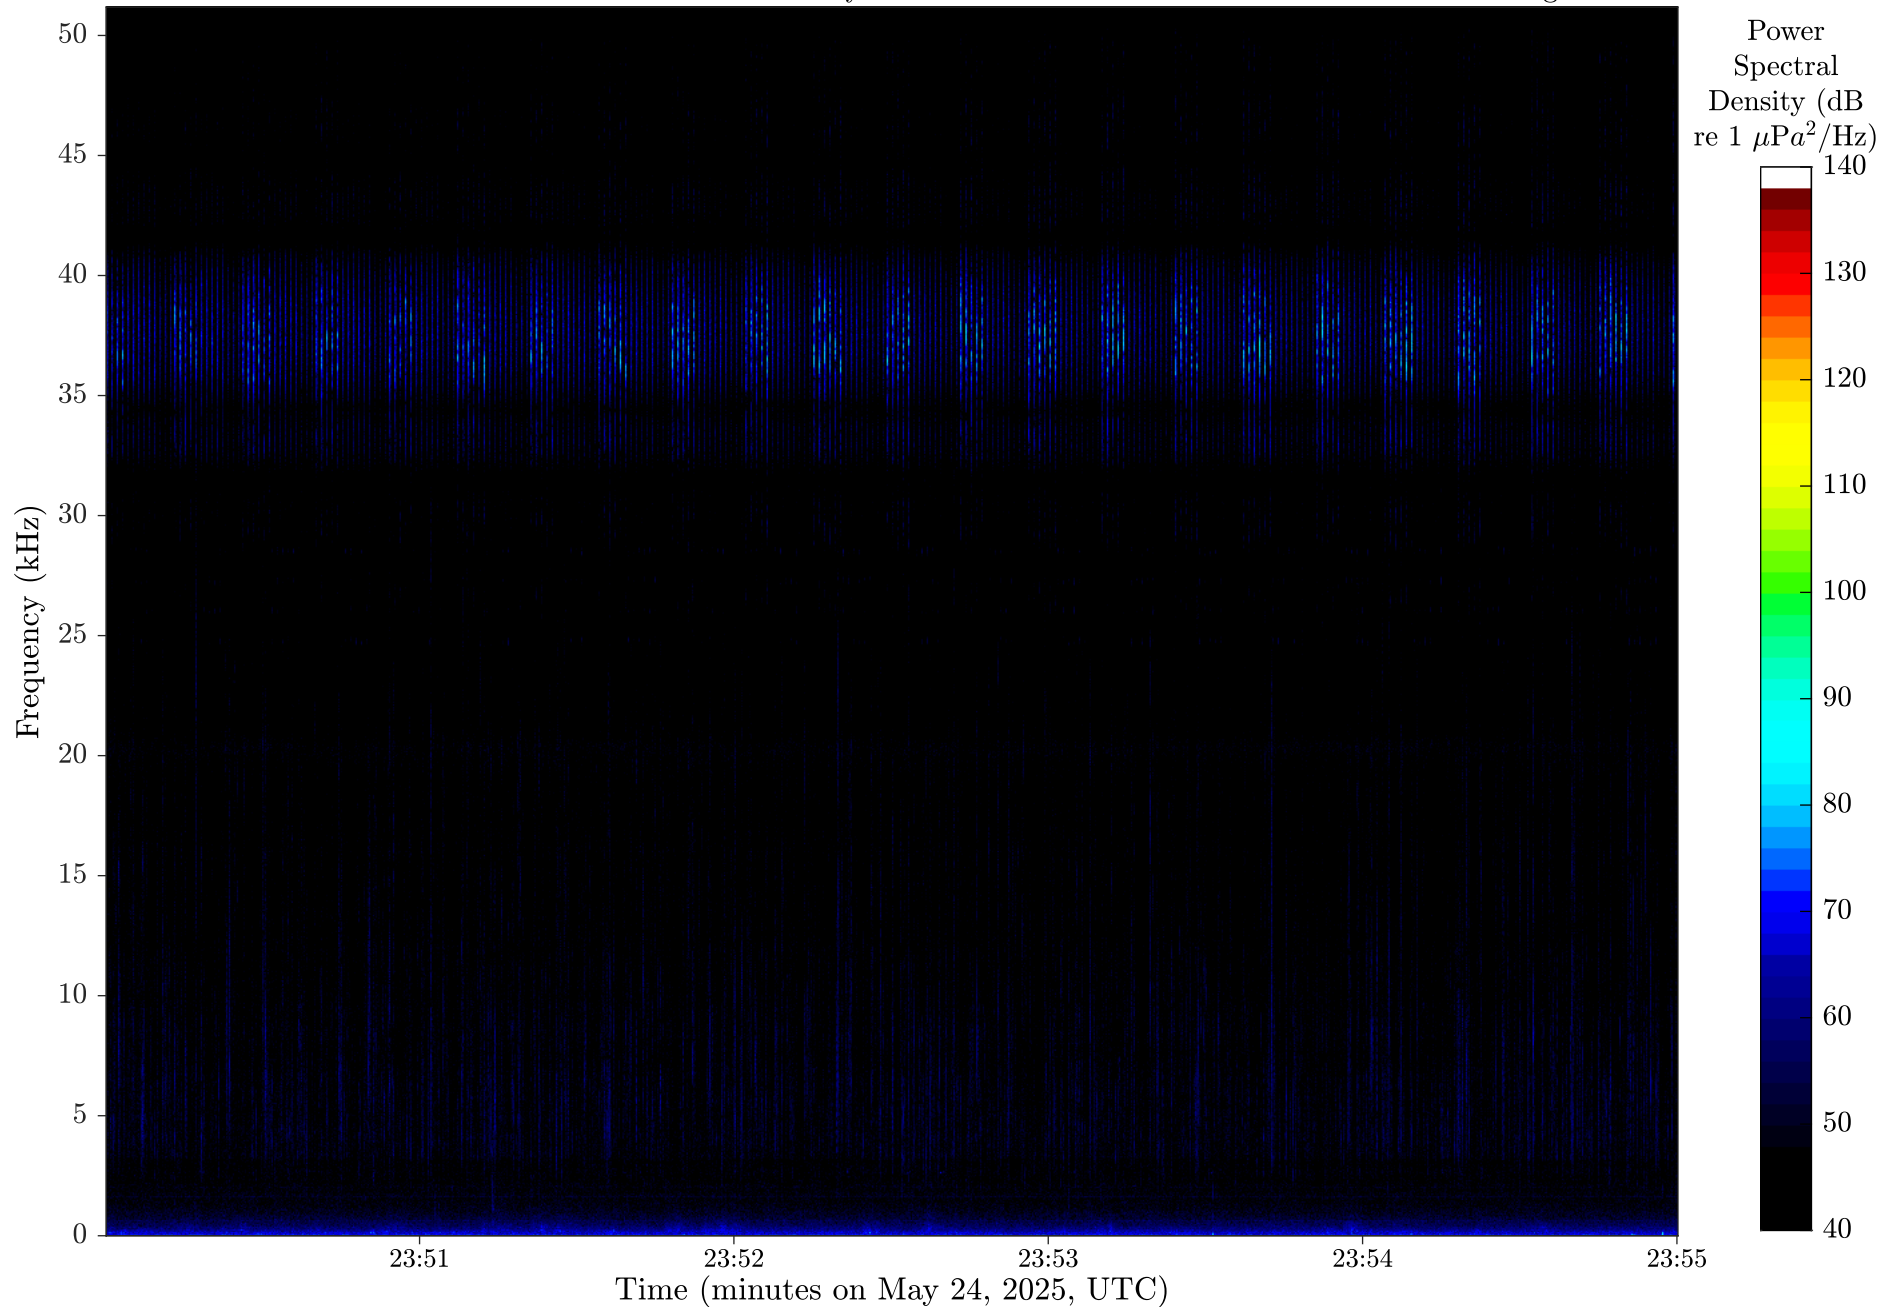

Comments: 34.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:54:50 UTC

