



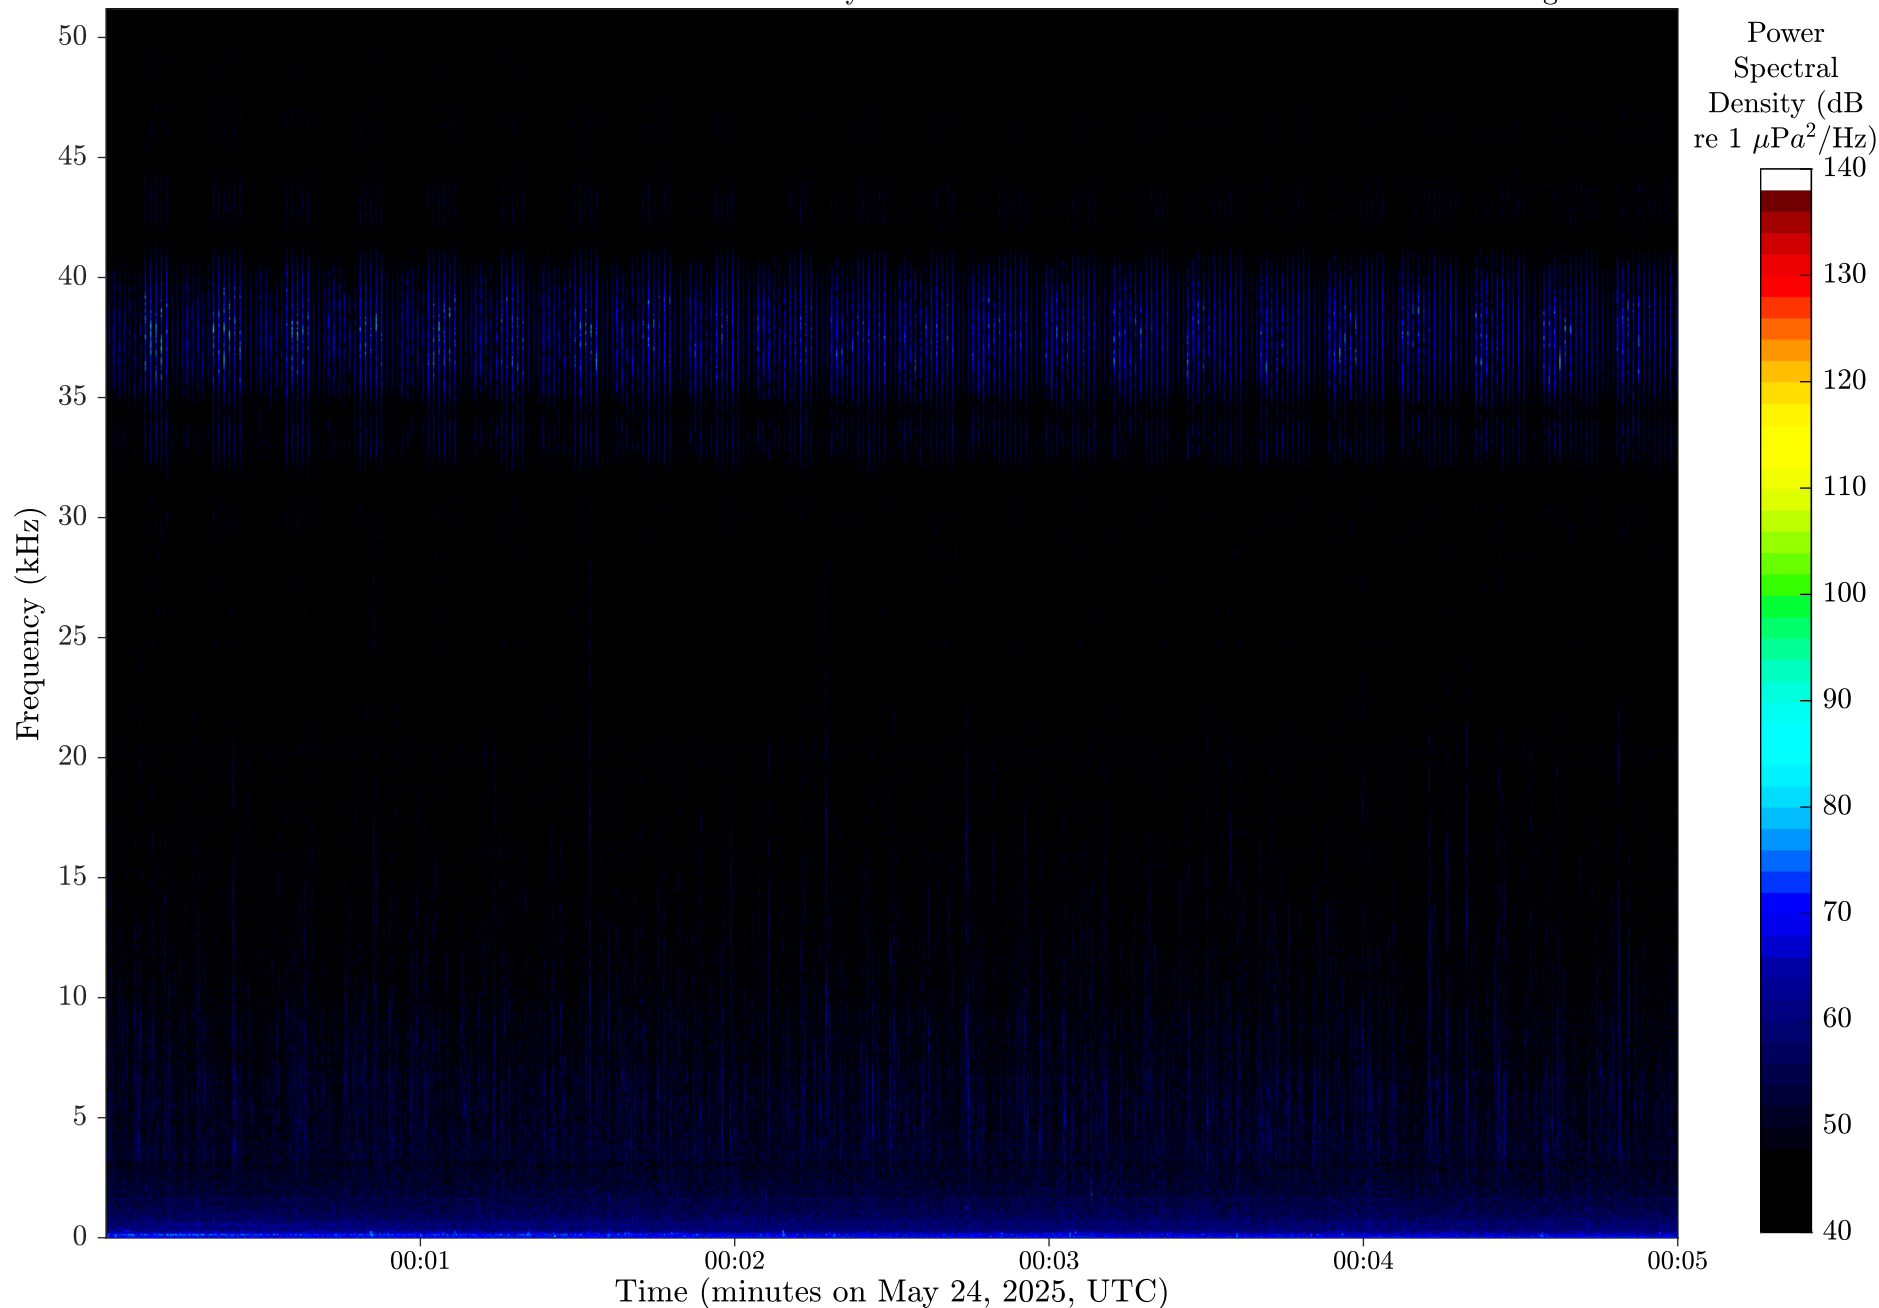


Comments: 31.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:18:47 UTC

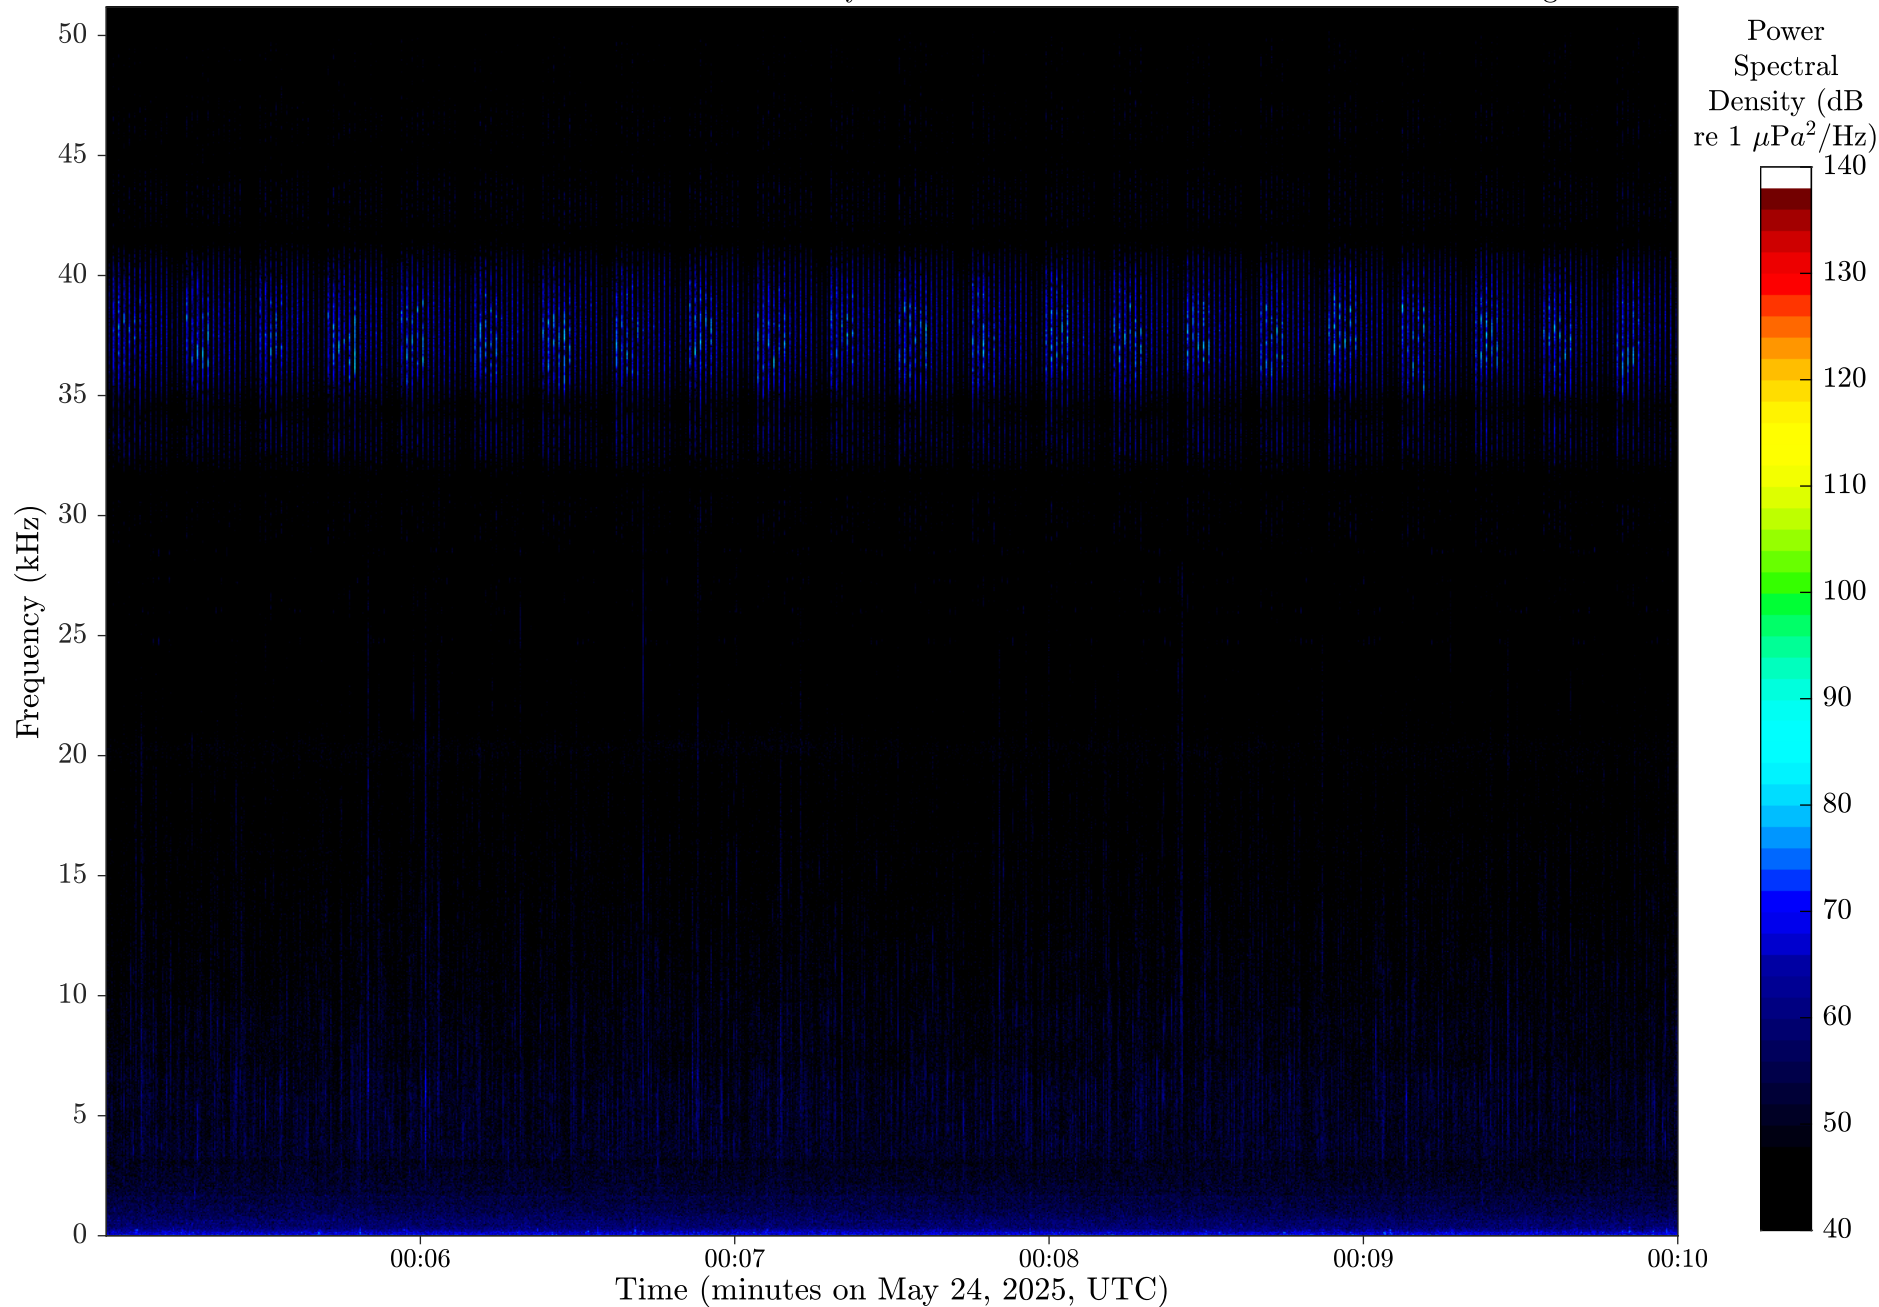


Comments: 32.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:18:57 UTC

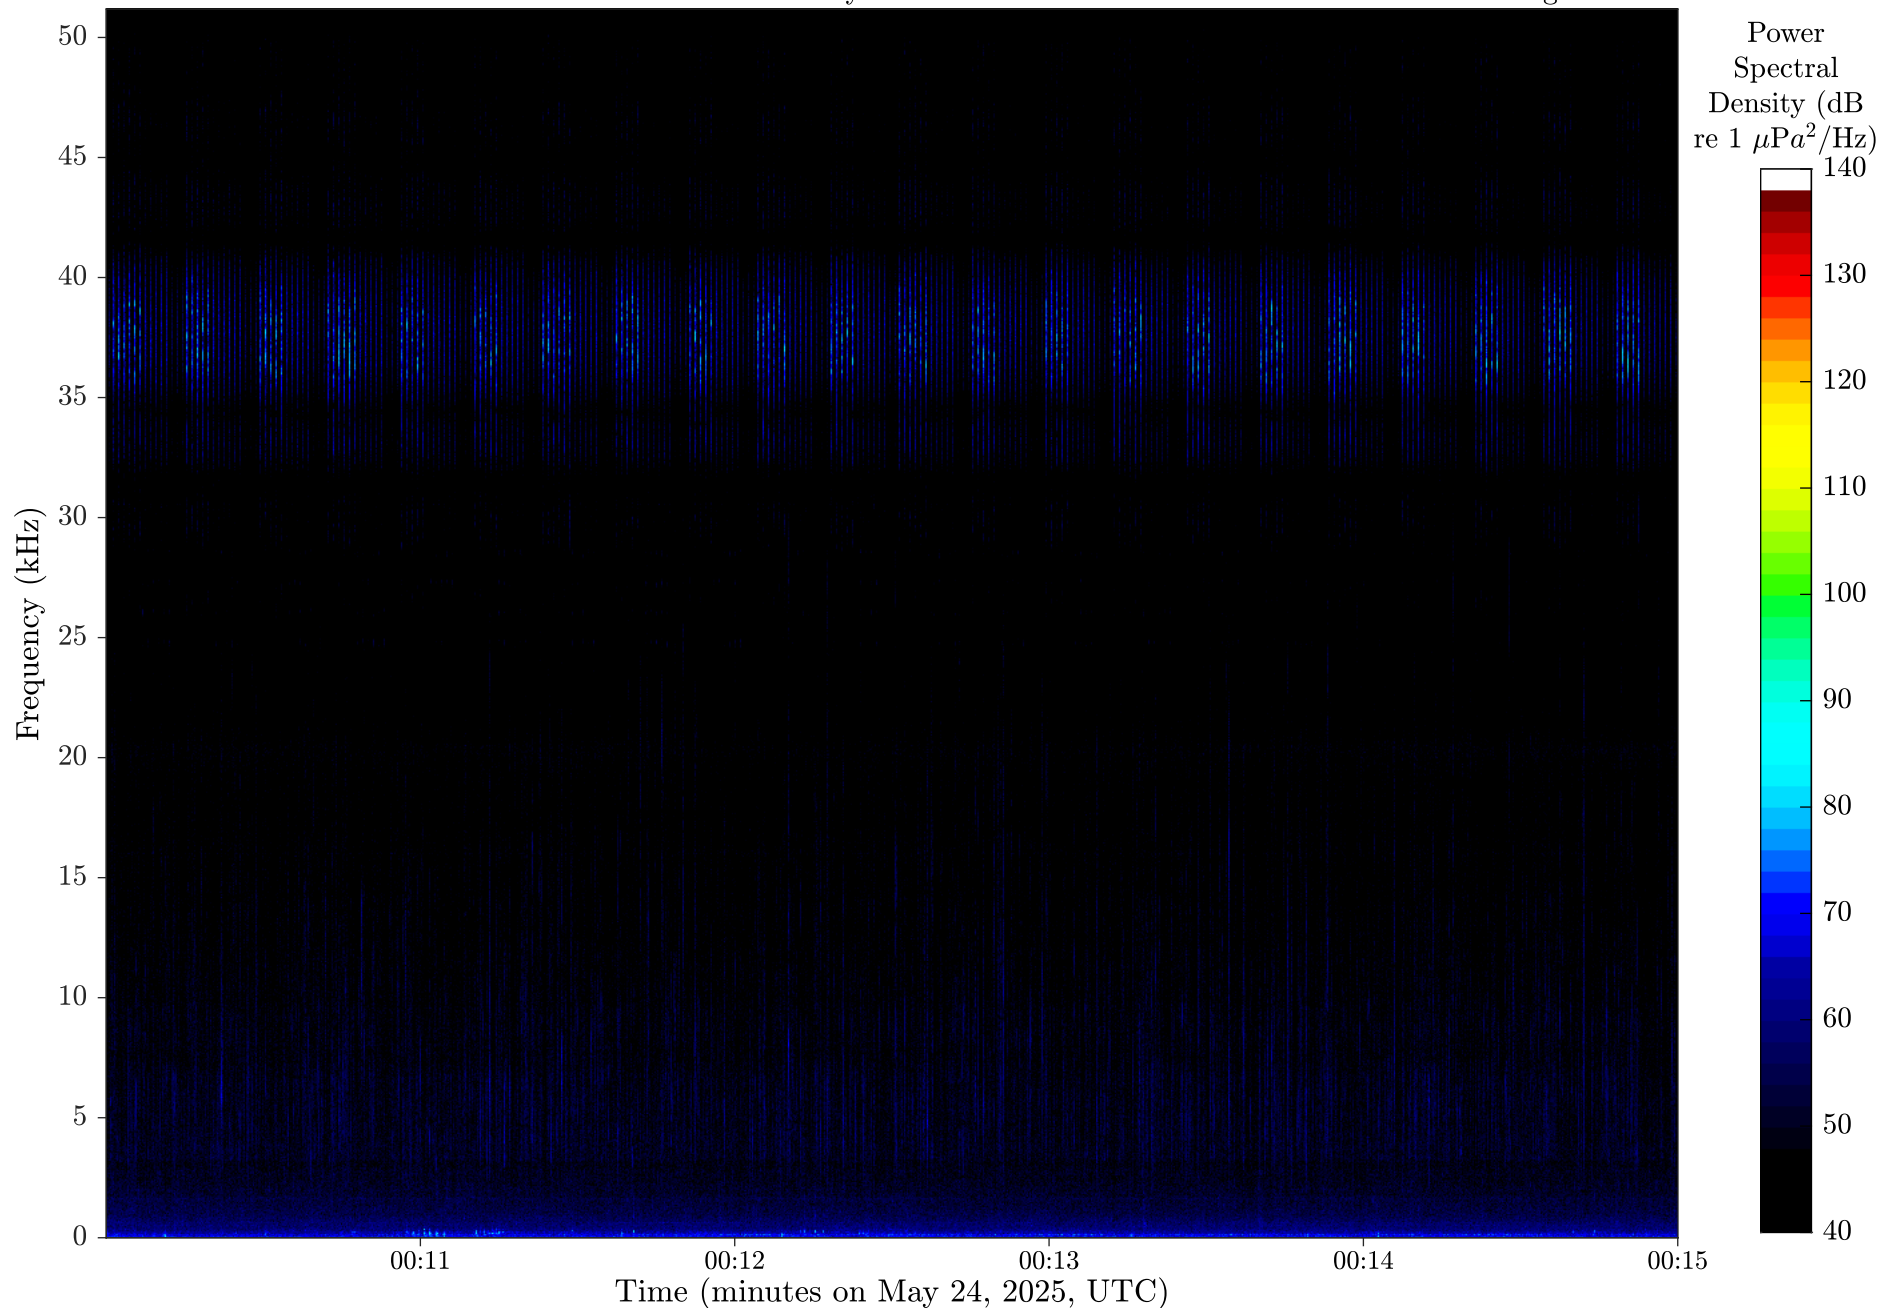


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:19:06 UTC

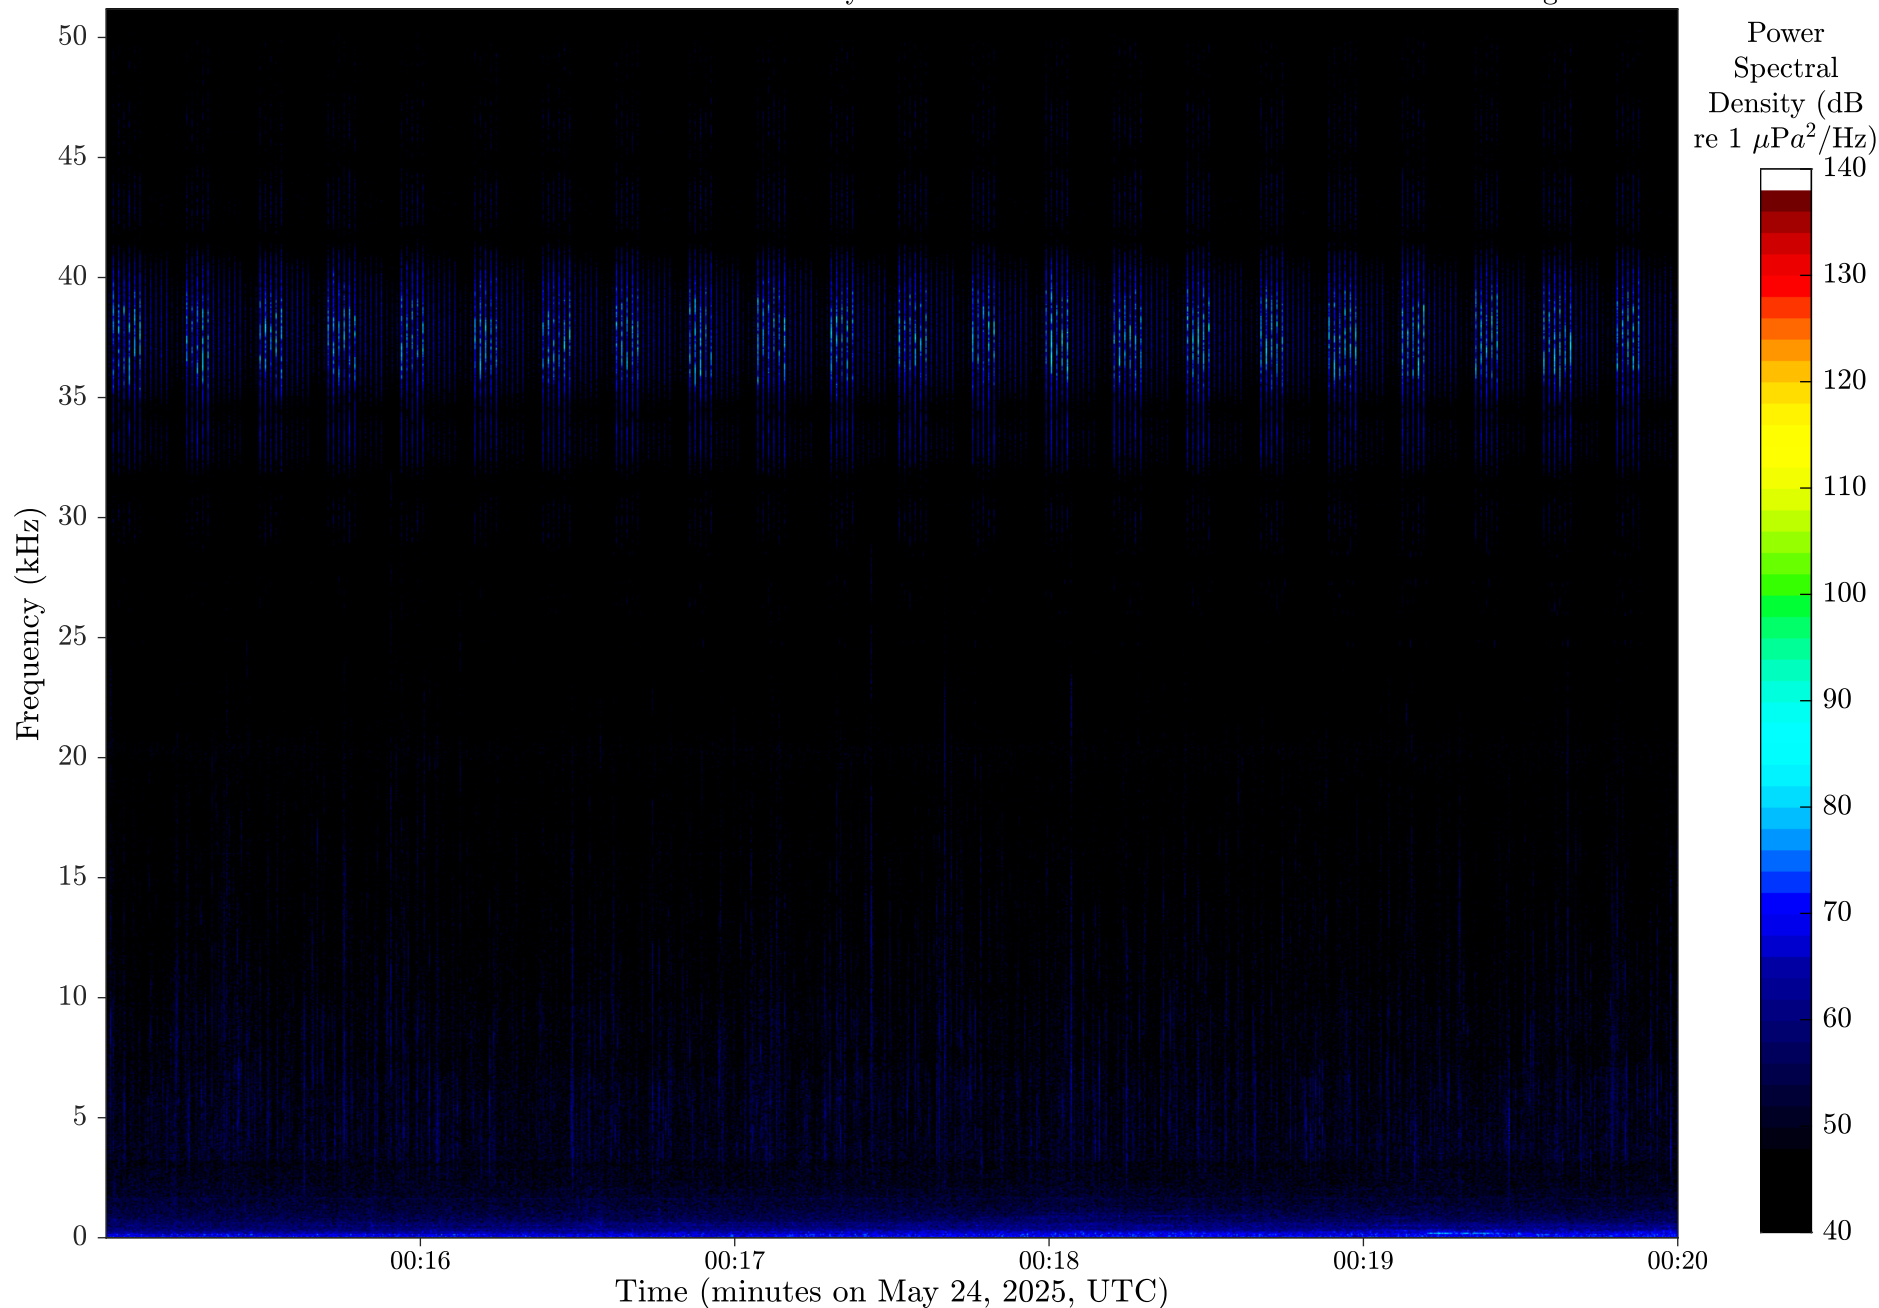


Comments: 35.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:19:15 UTC

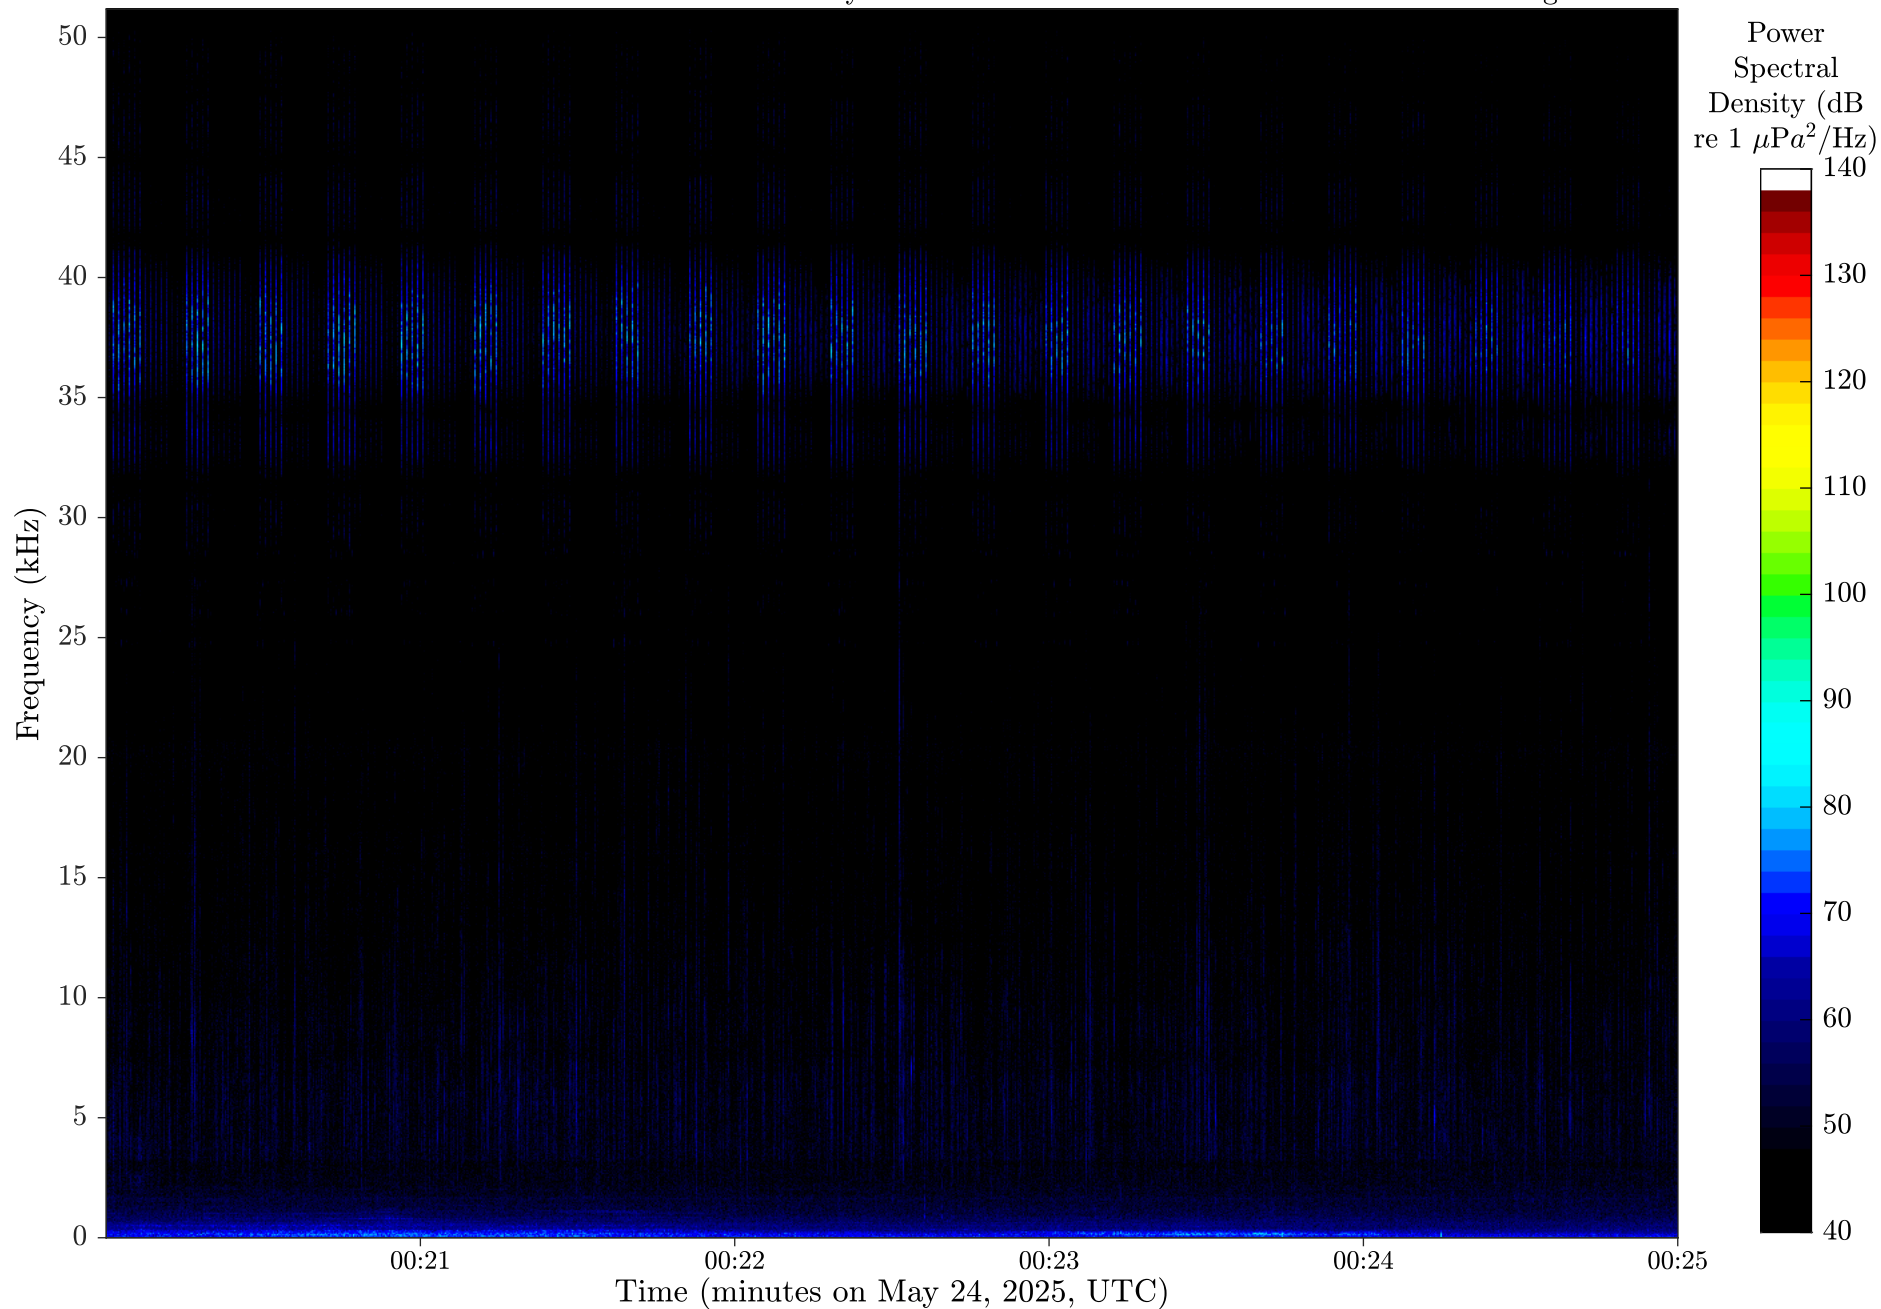

Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:19:25 UTC

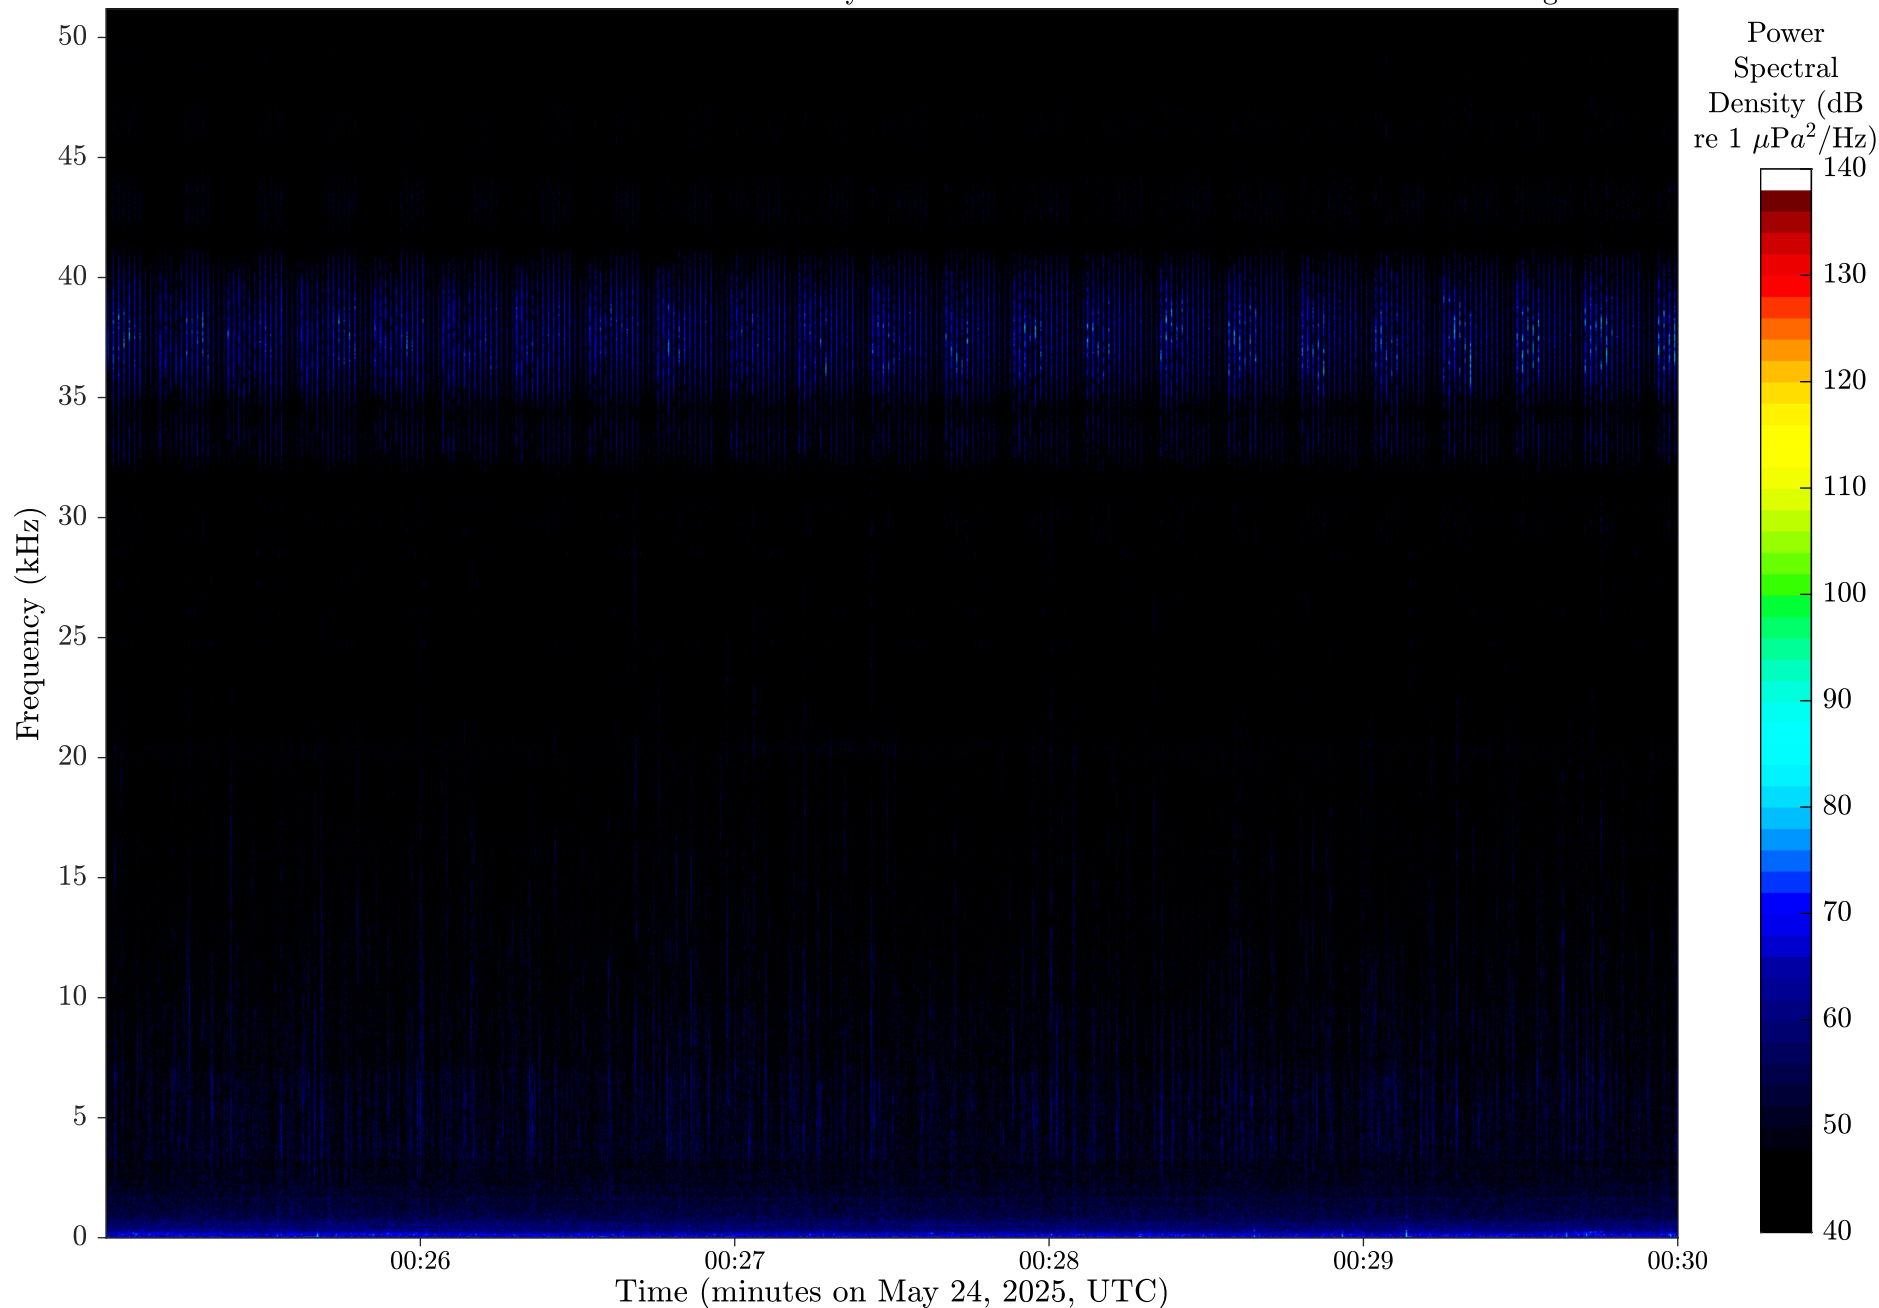

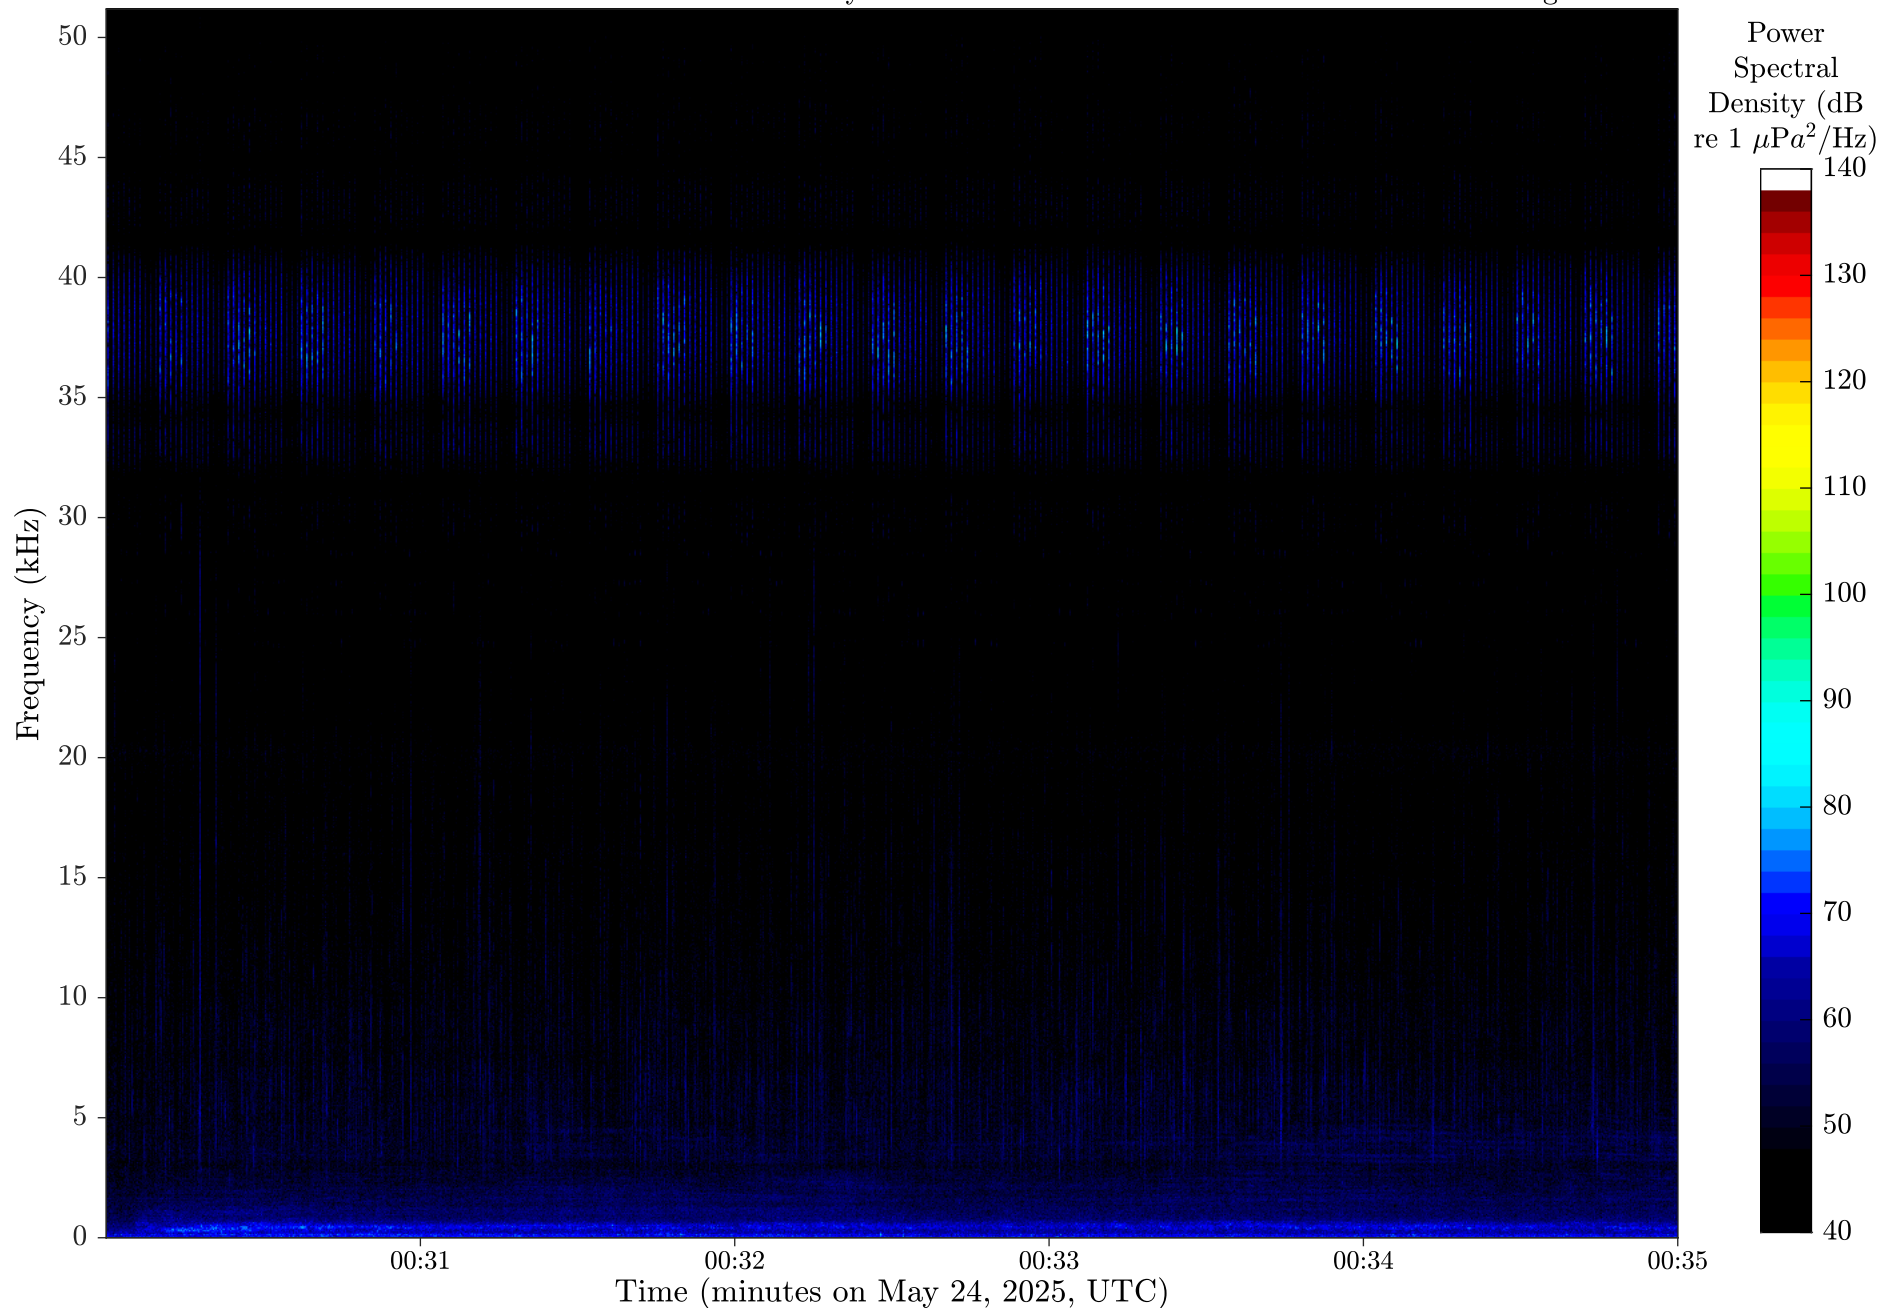


Comments: 33.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:19:43 UTC

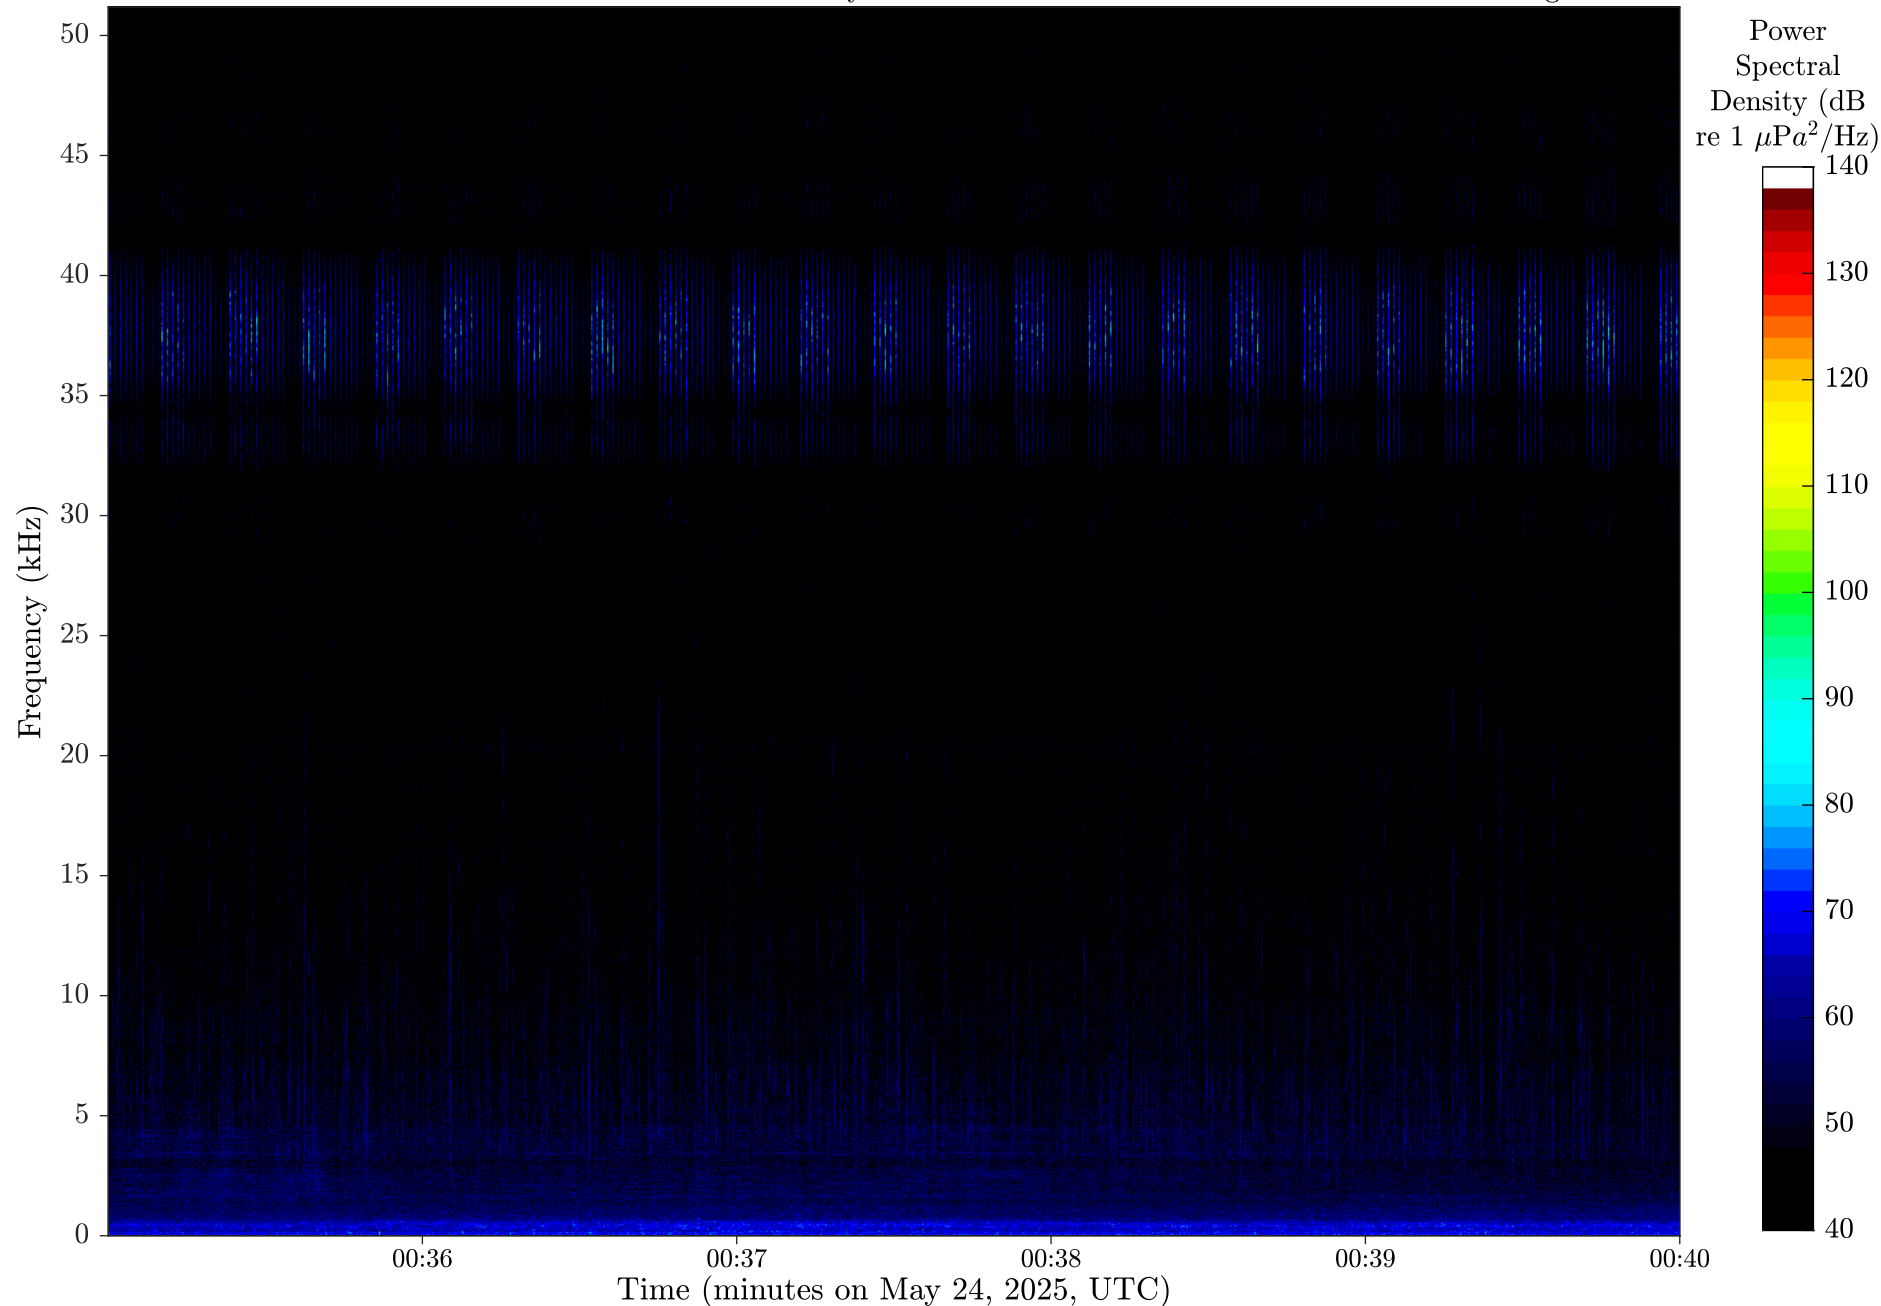


Comments: 34.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:19:51 UTC

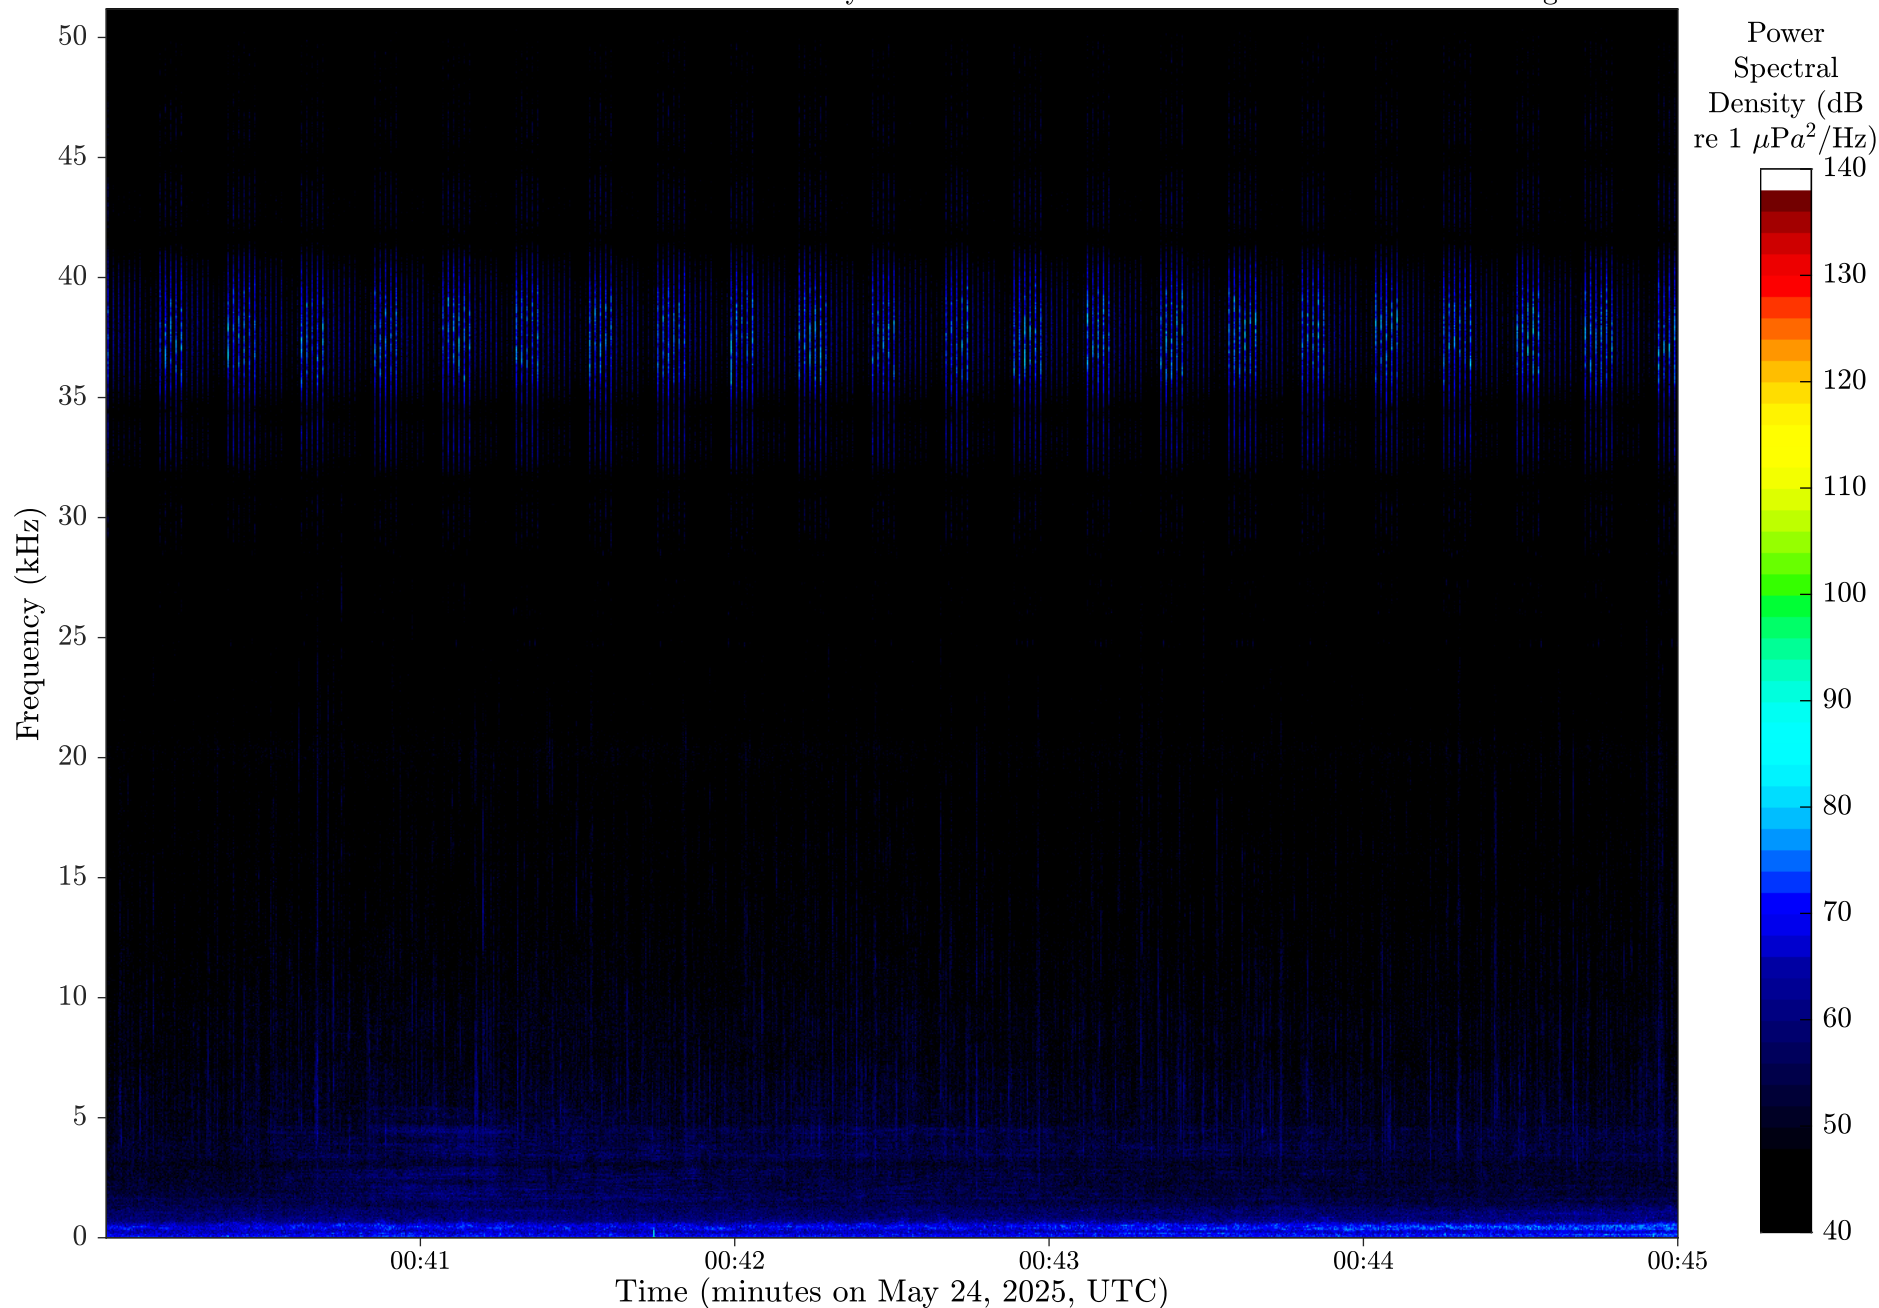

Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:19:59 UTC

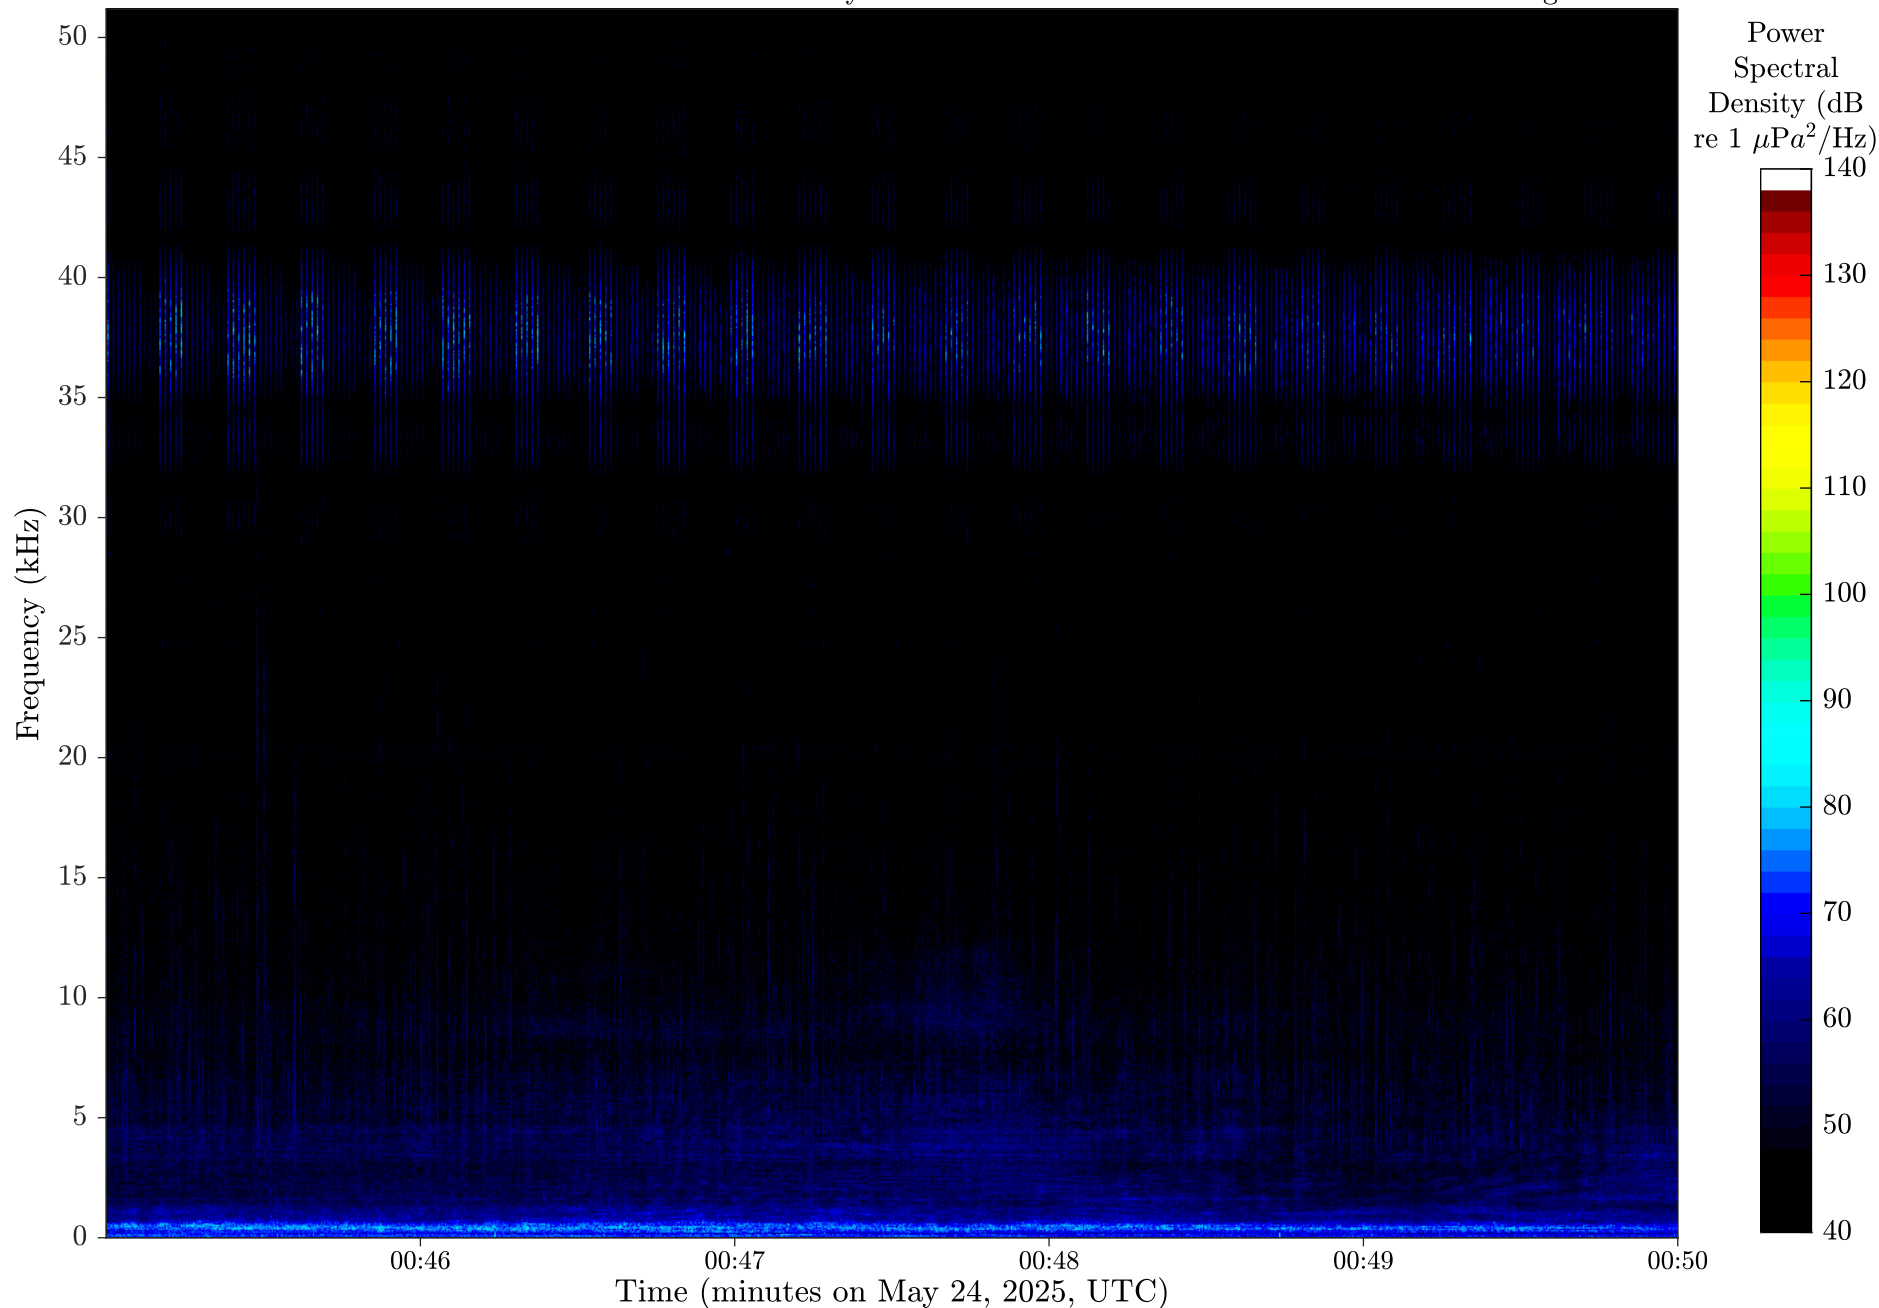

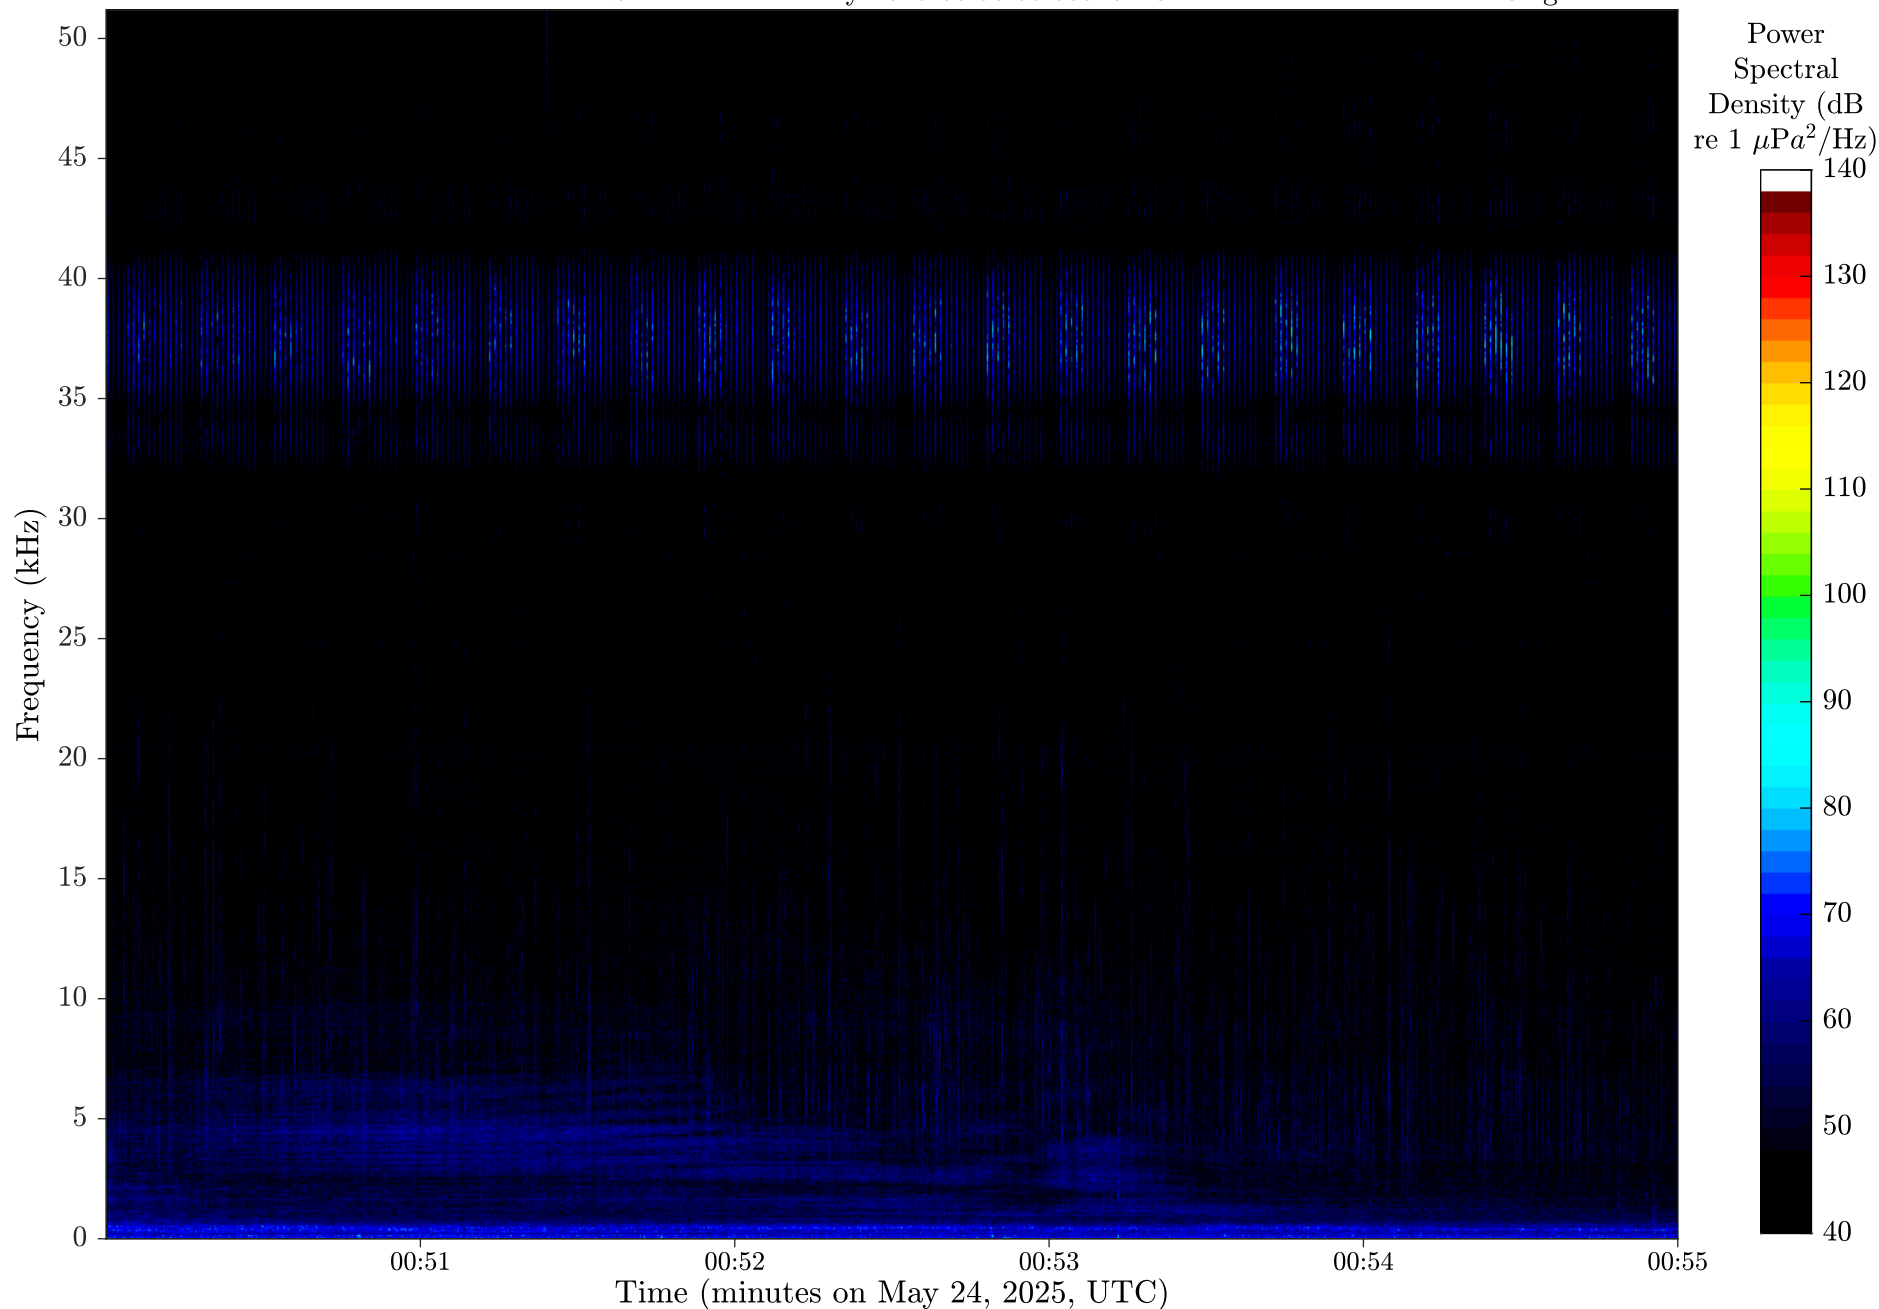


Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:16 UTC

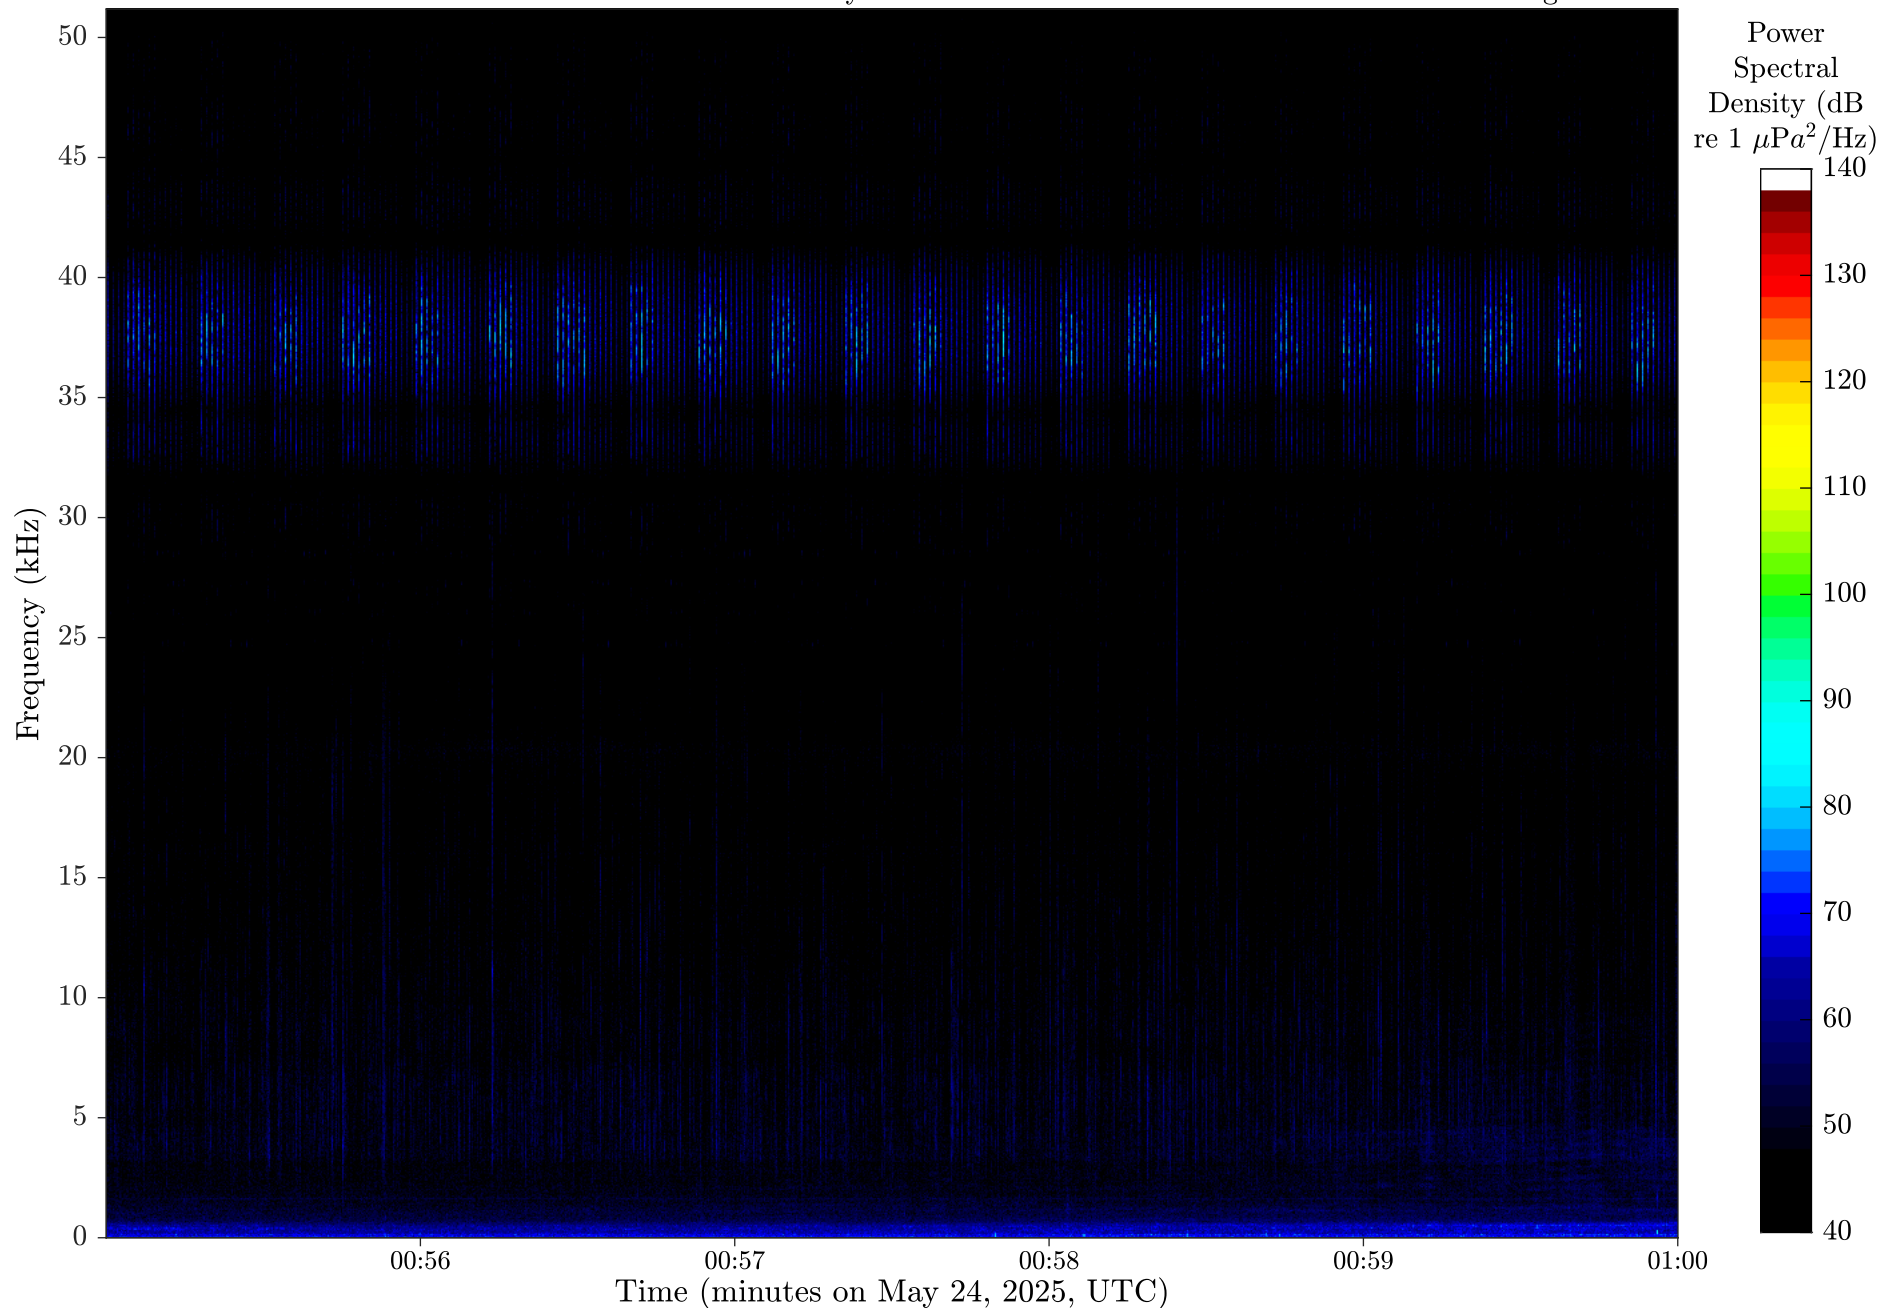


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:20:25 UTC

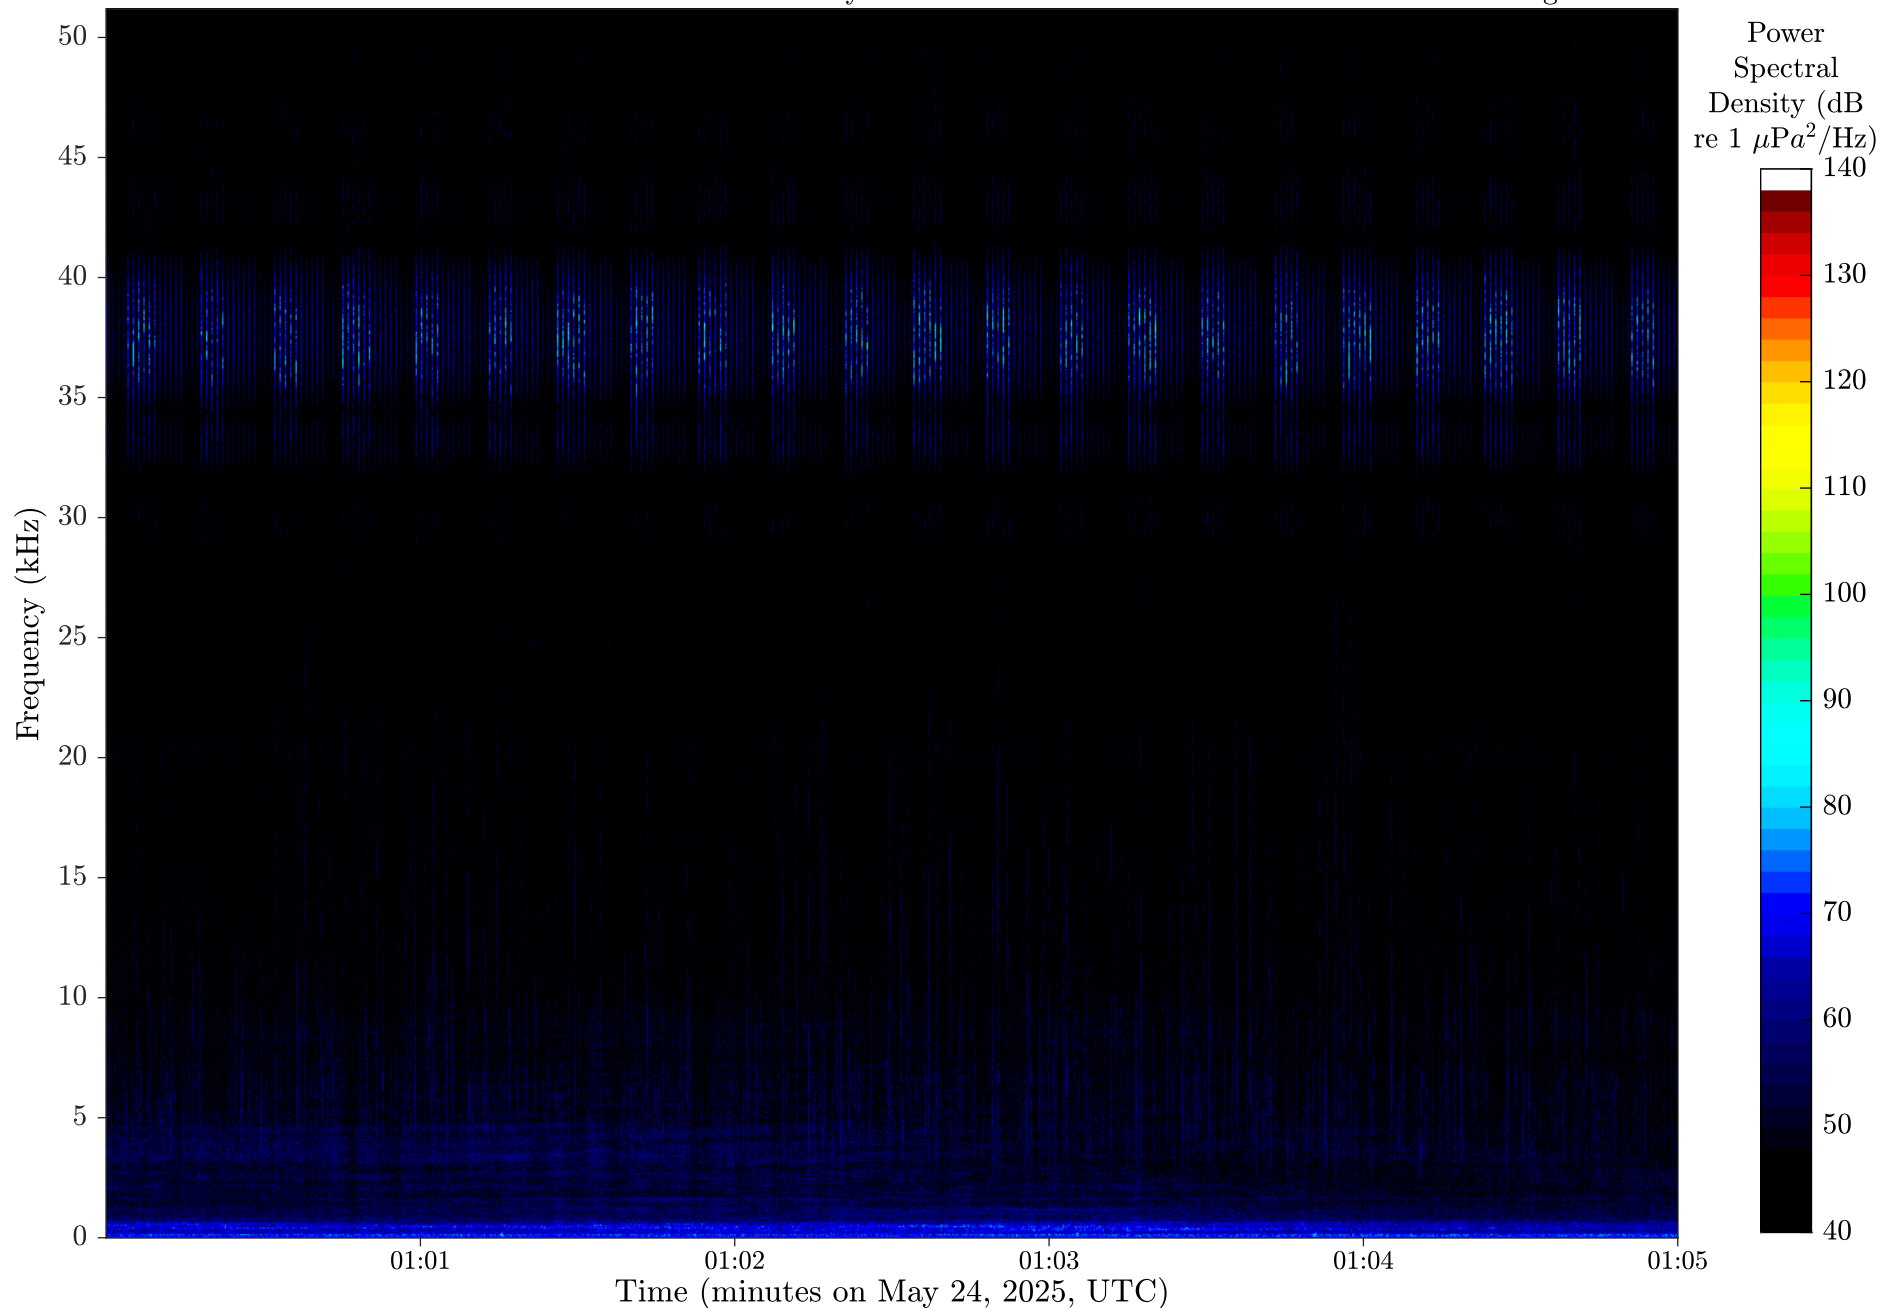


Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:20:34 UTC

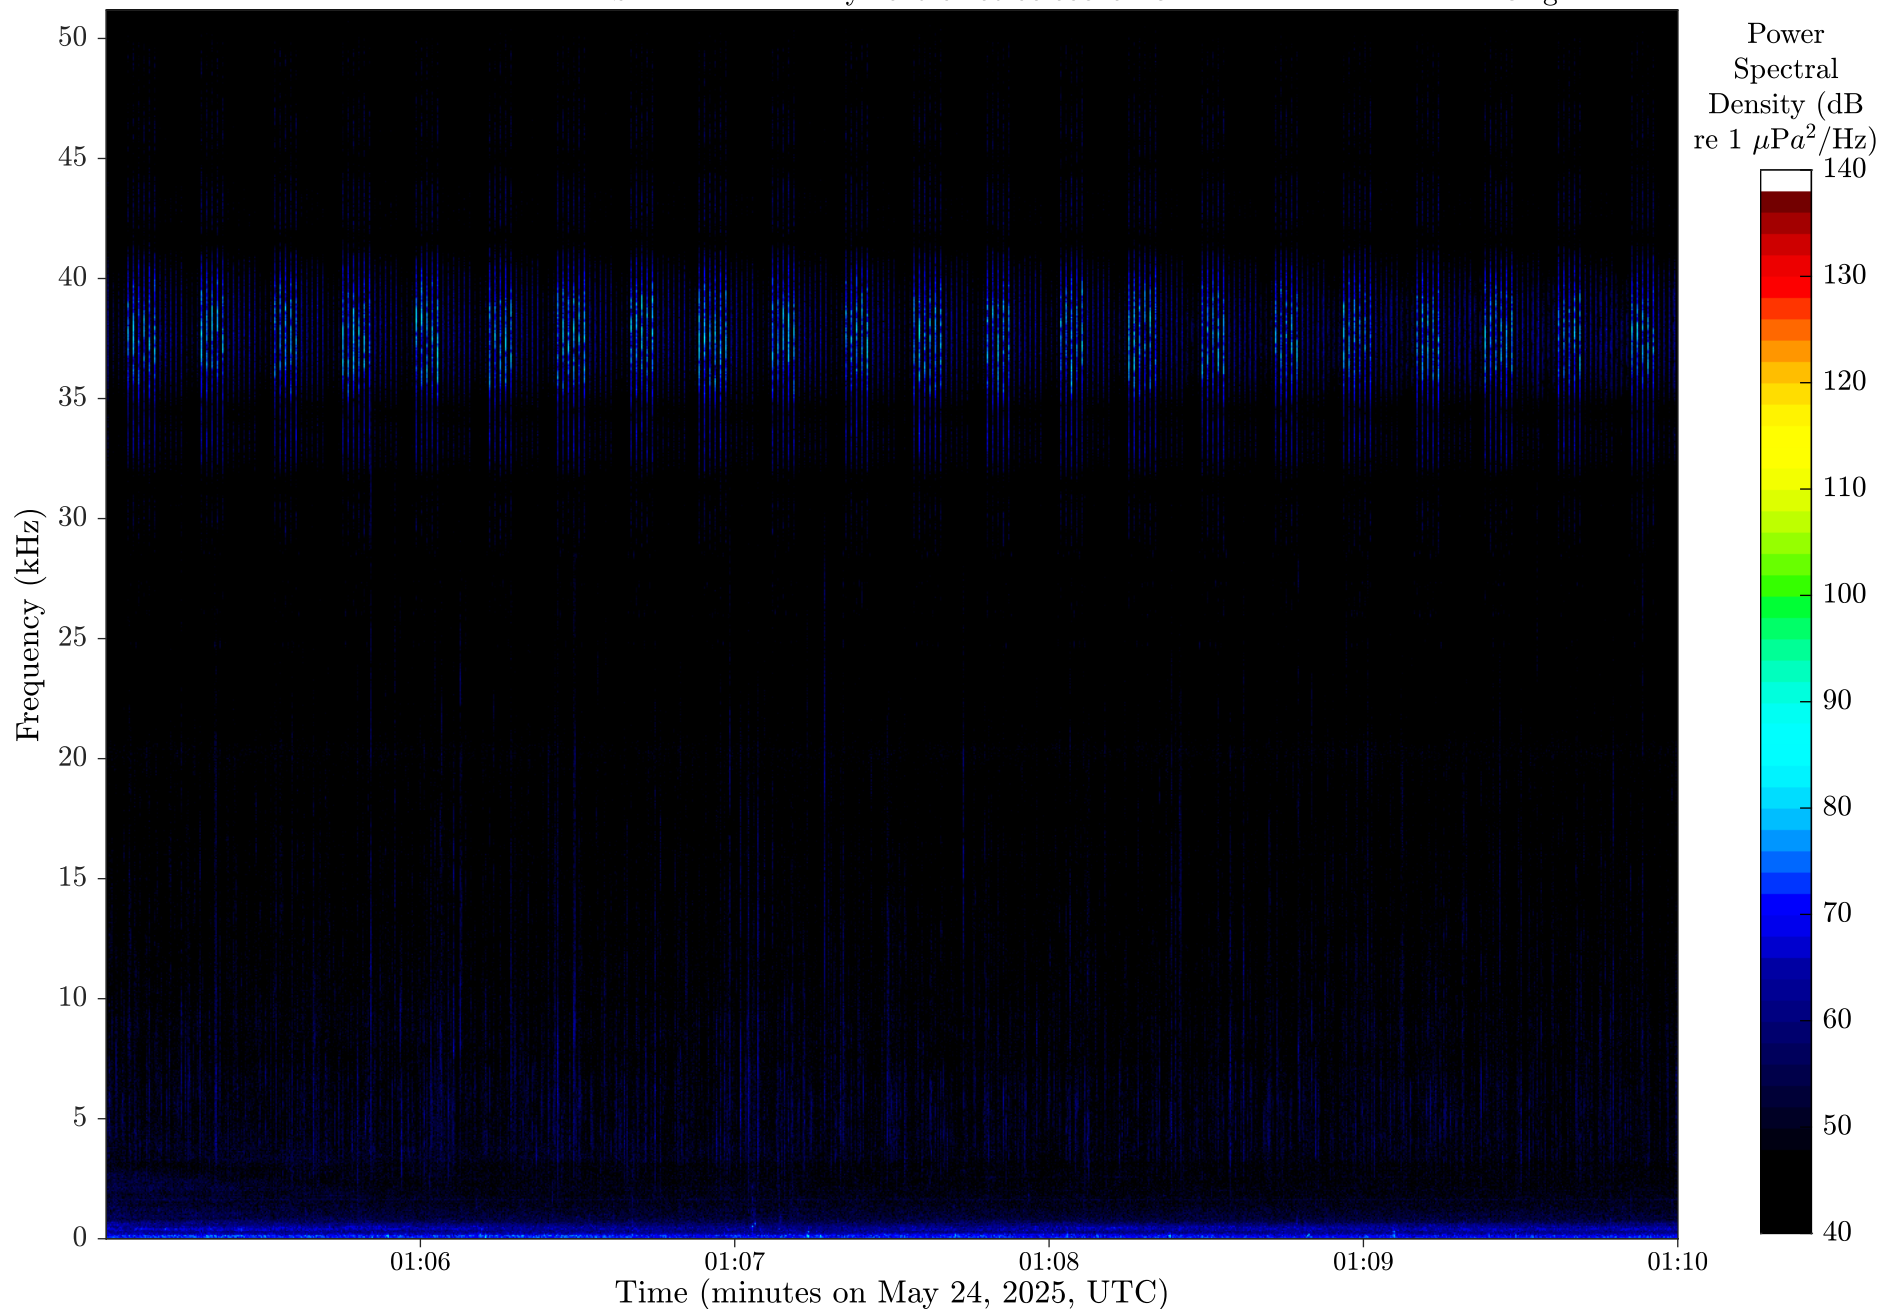

Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:20:42 UTC

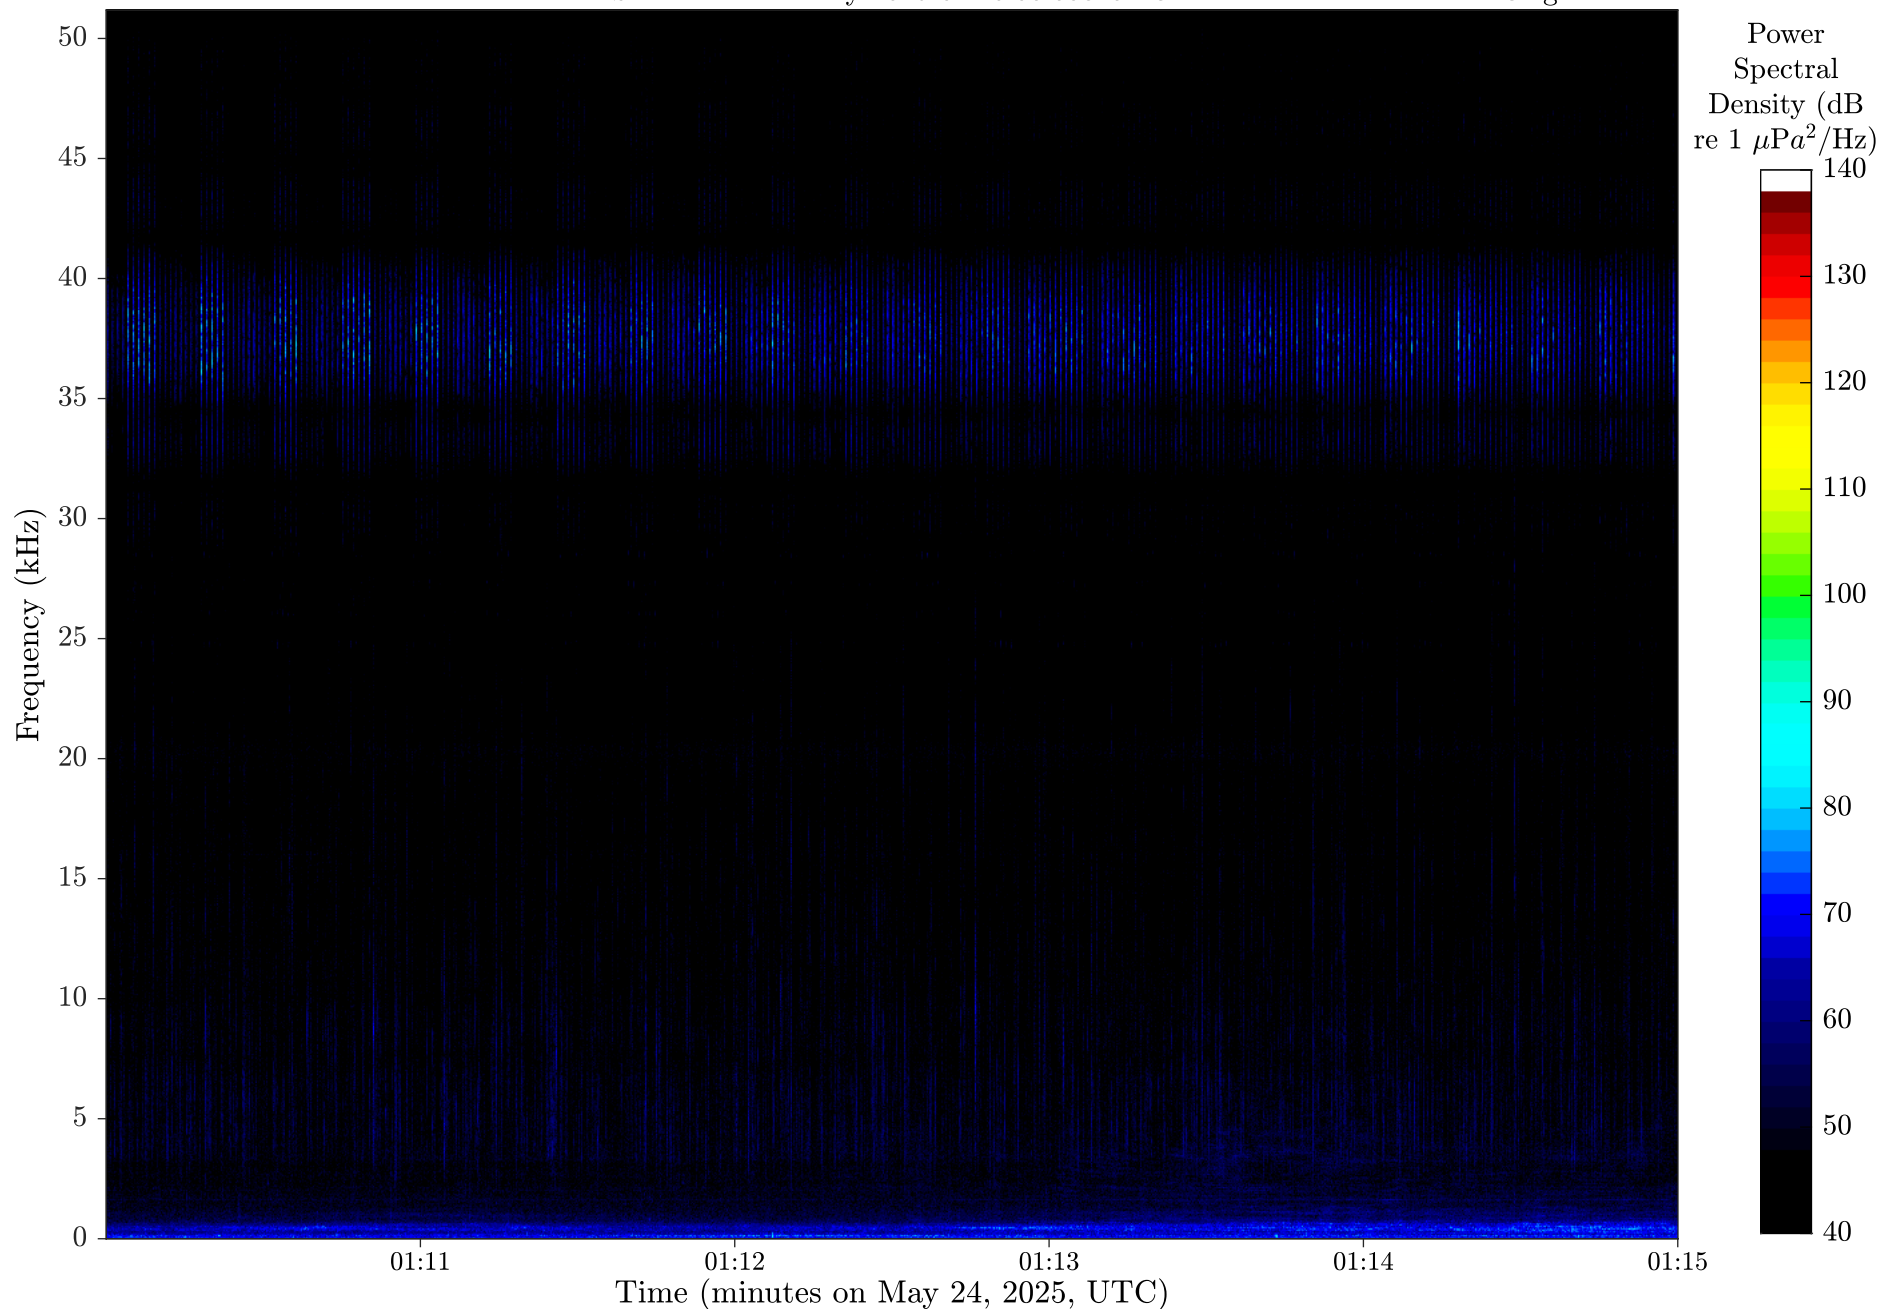

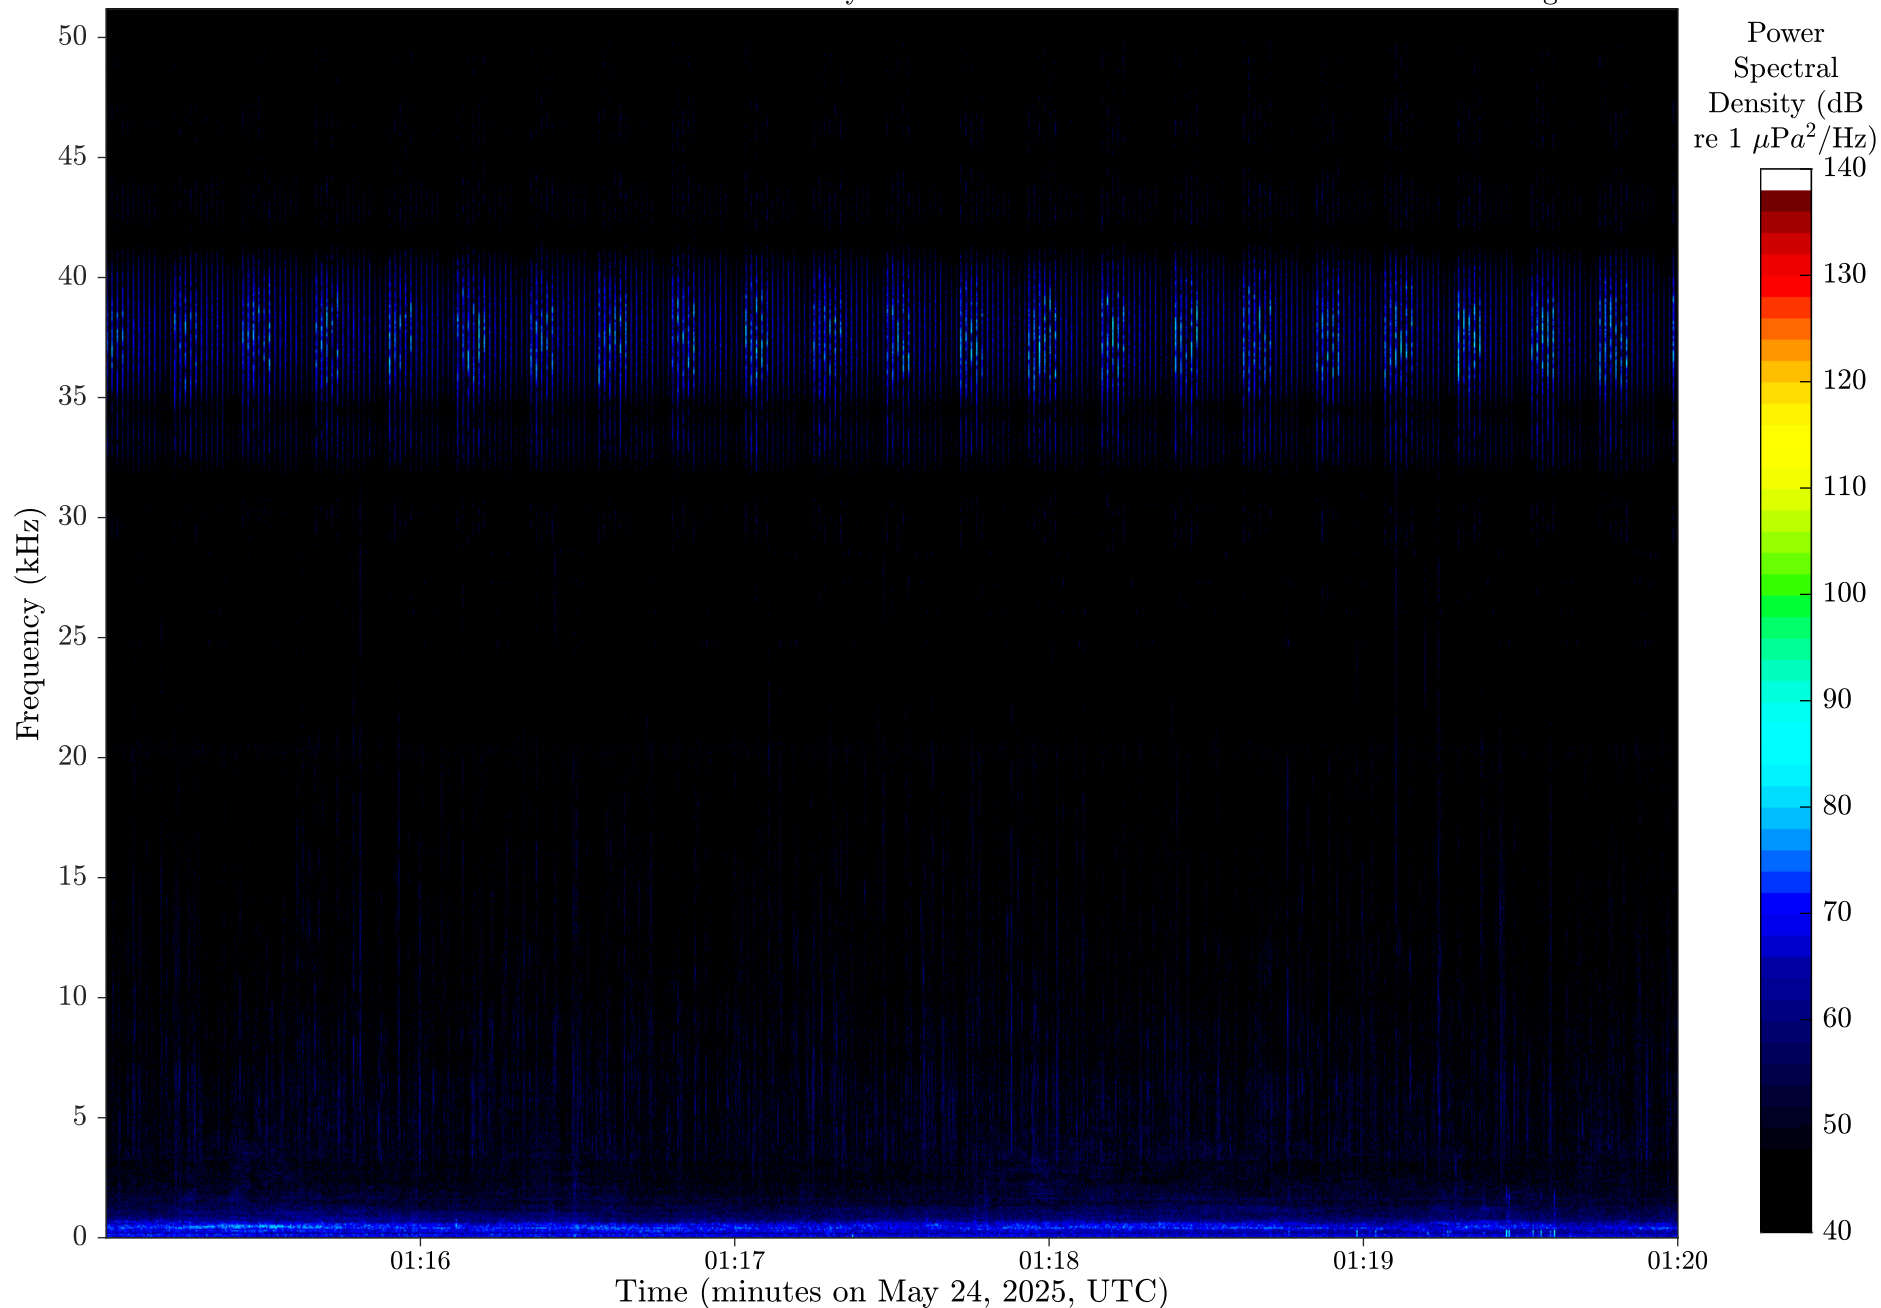


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:00 UTC

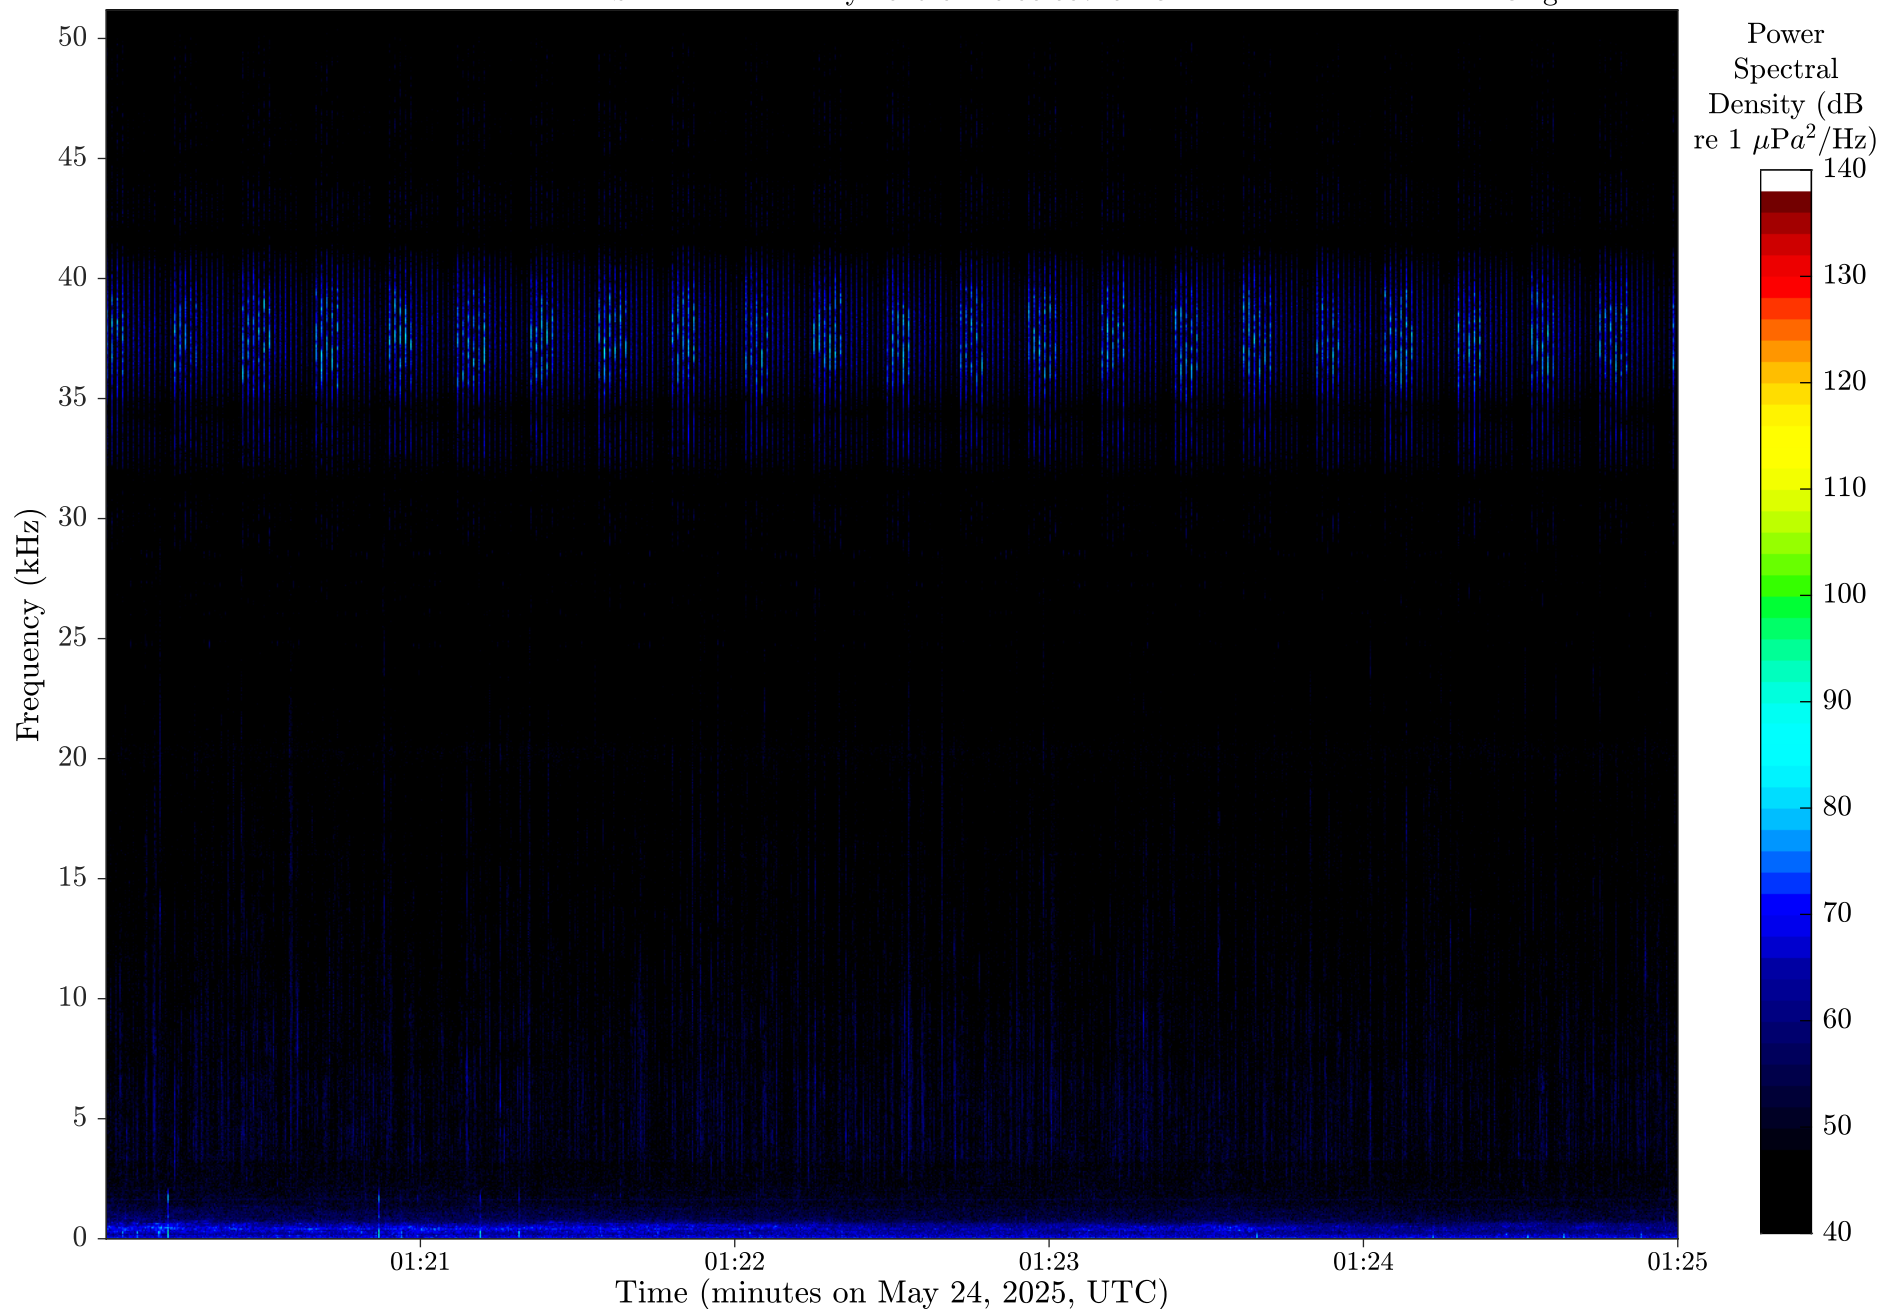


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:09 UTC

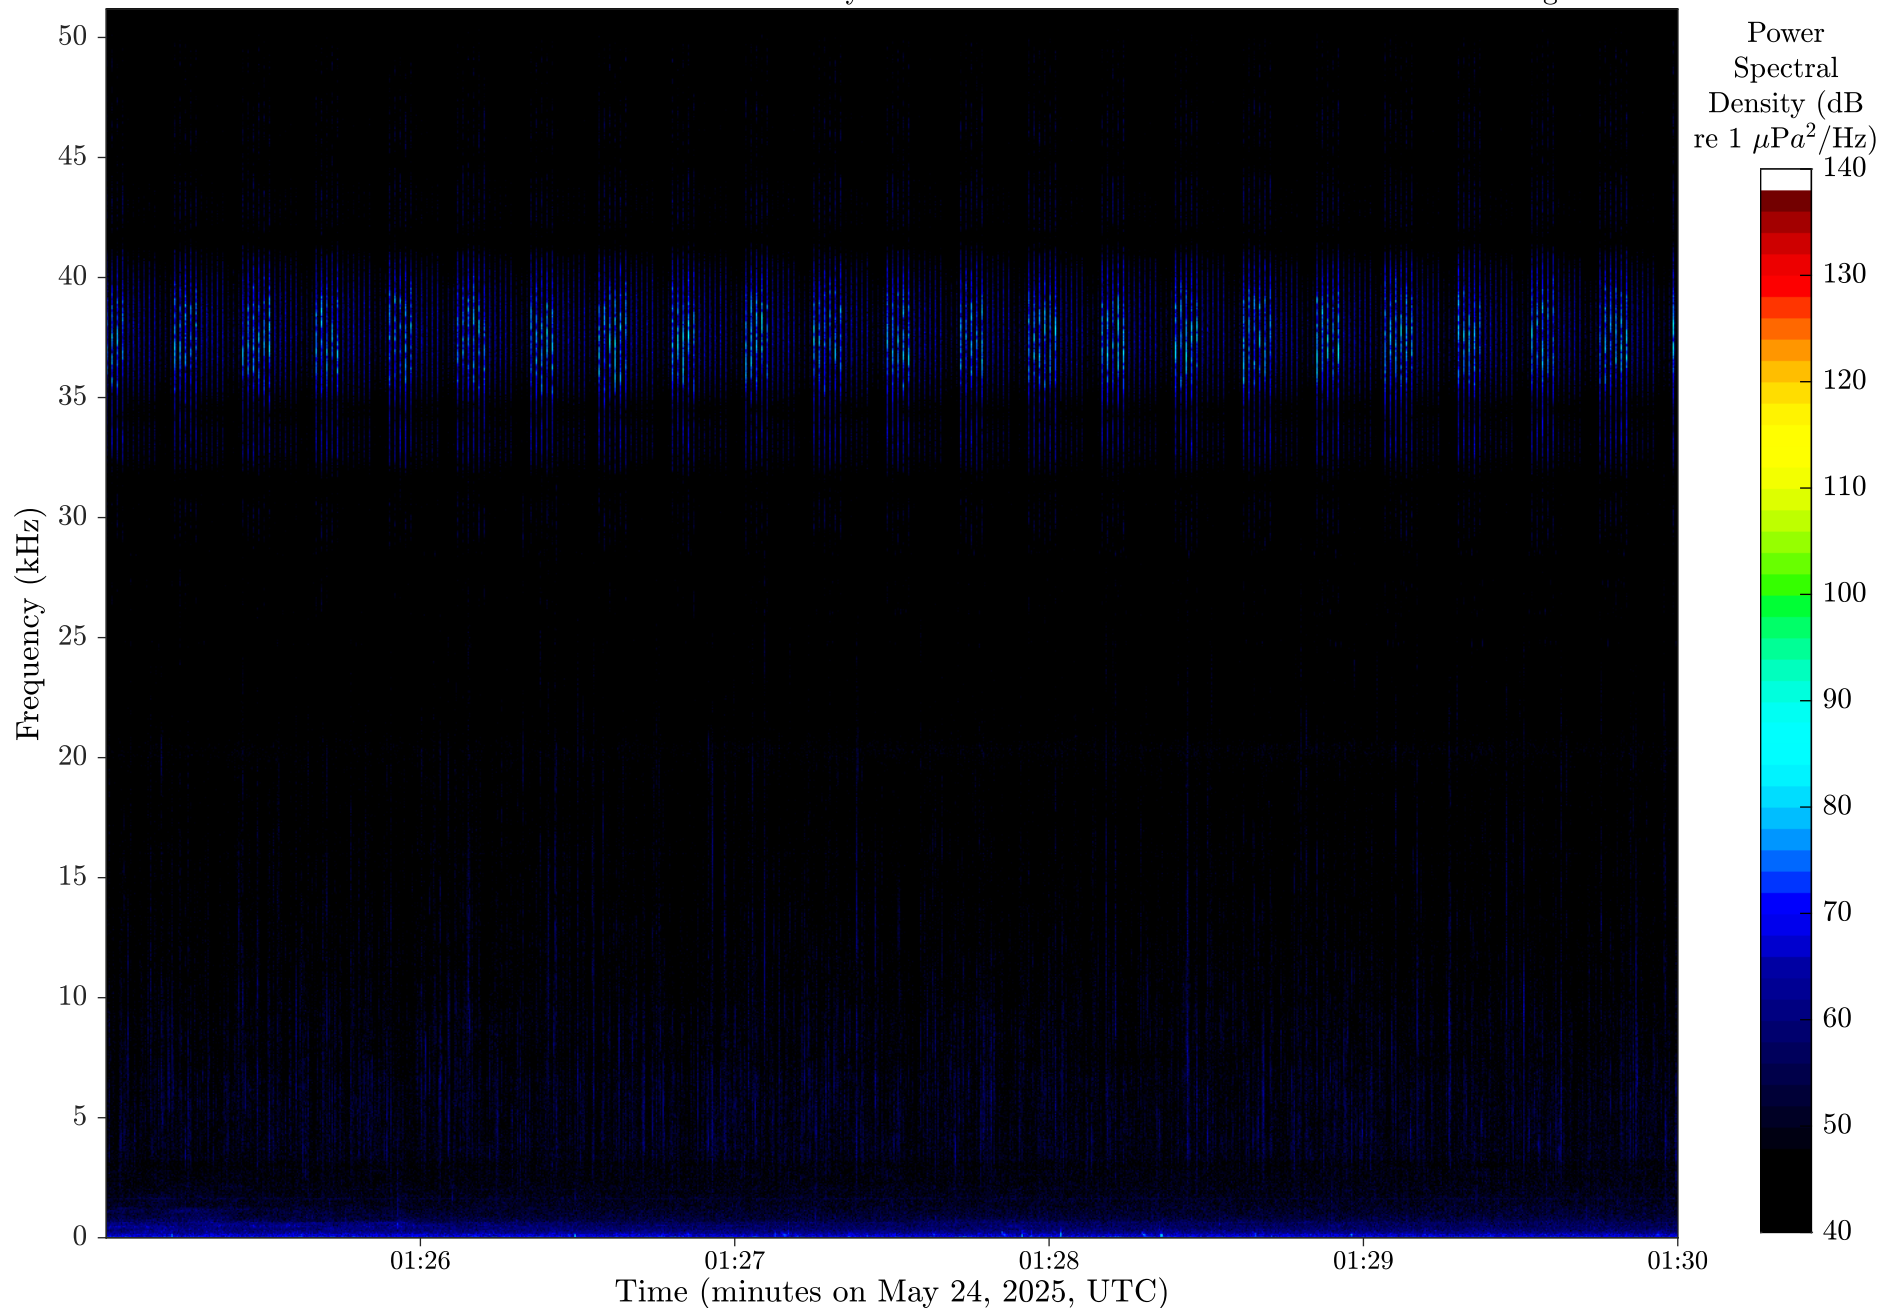


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:17 UTC

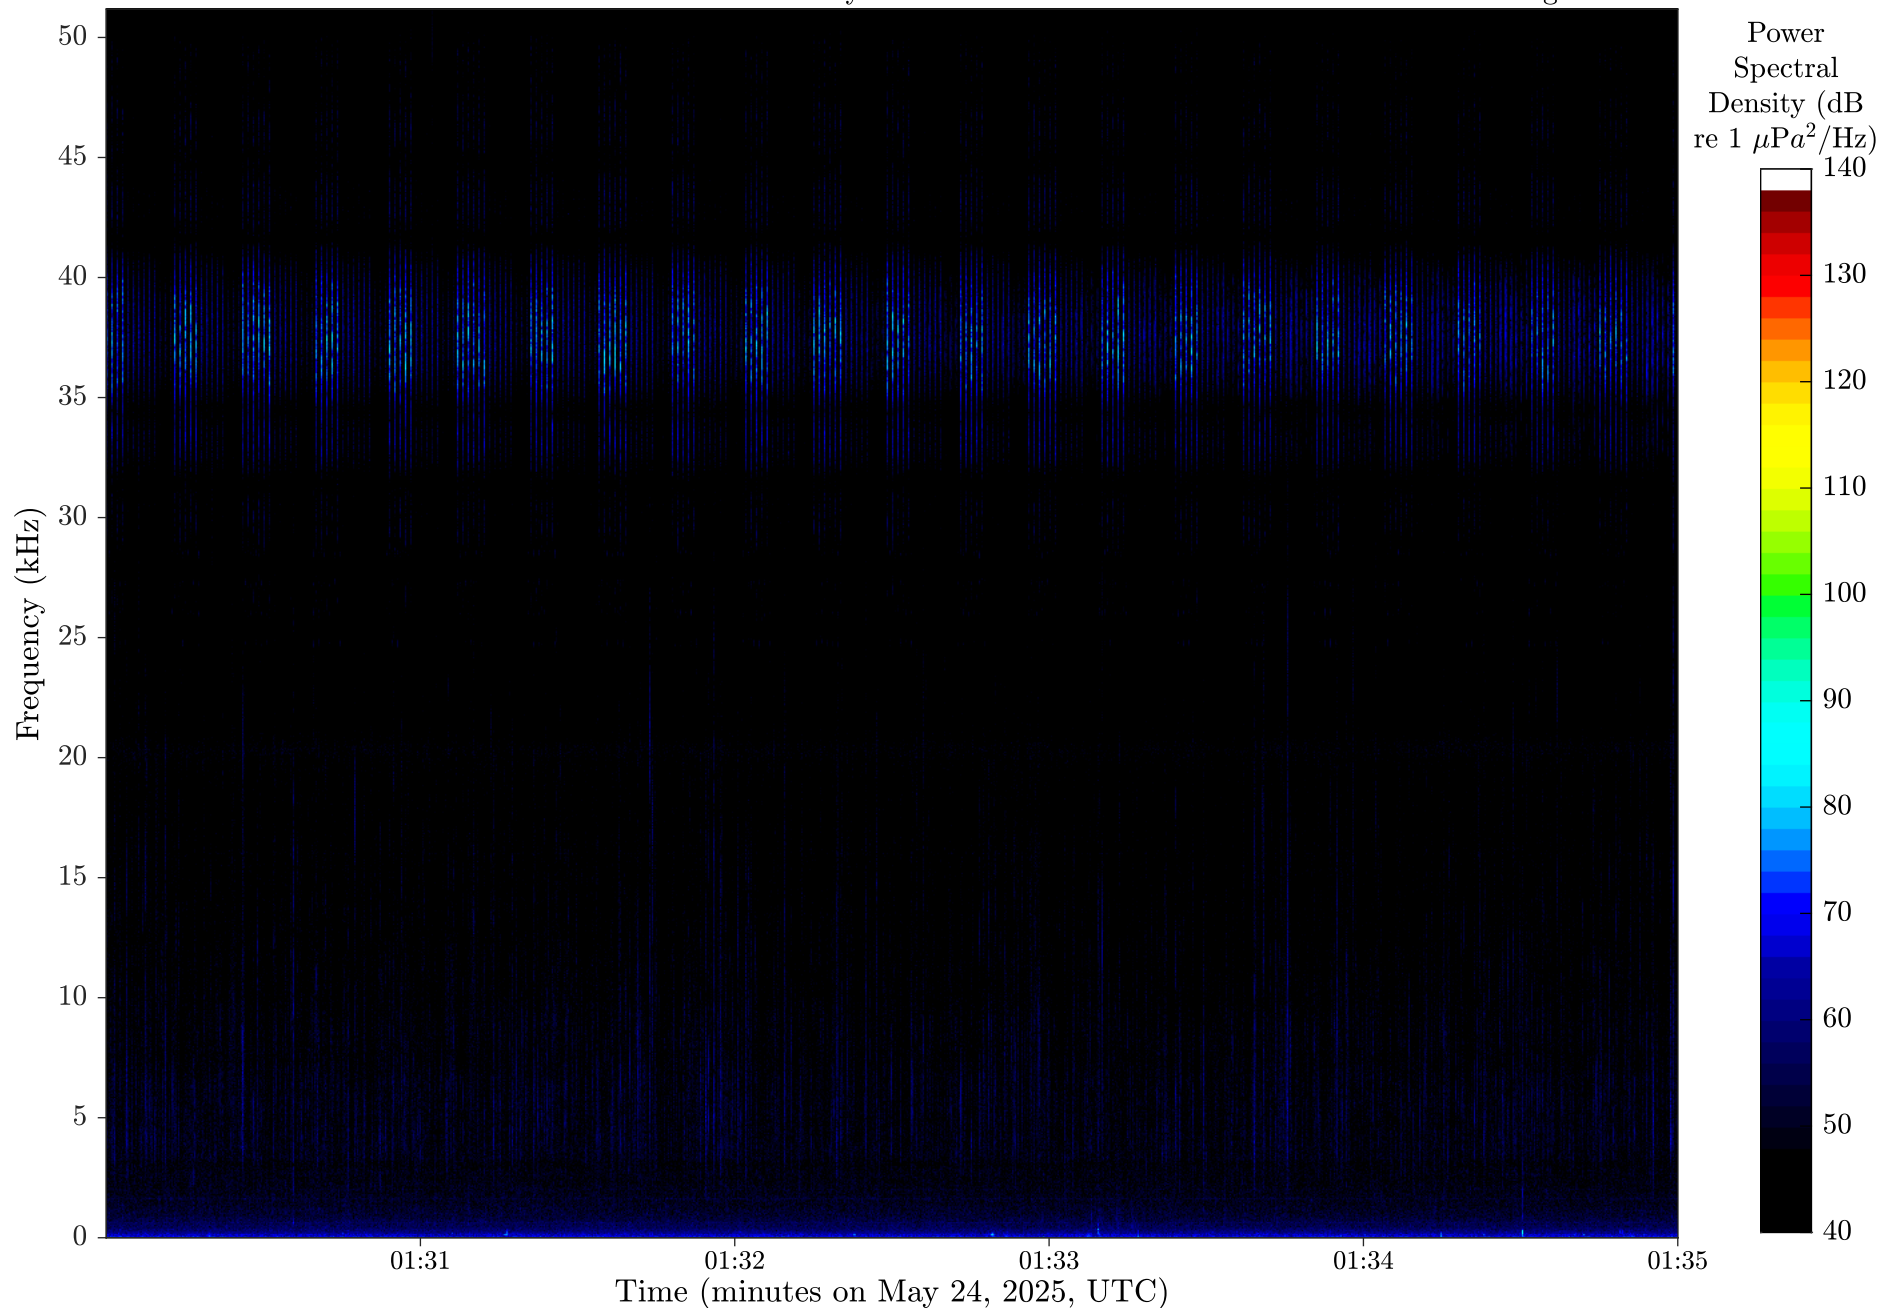


Comments: 34.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:25 UTC

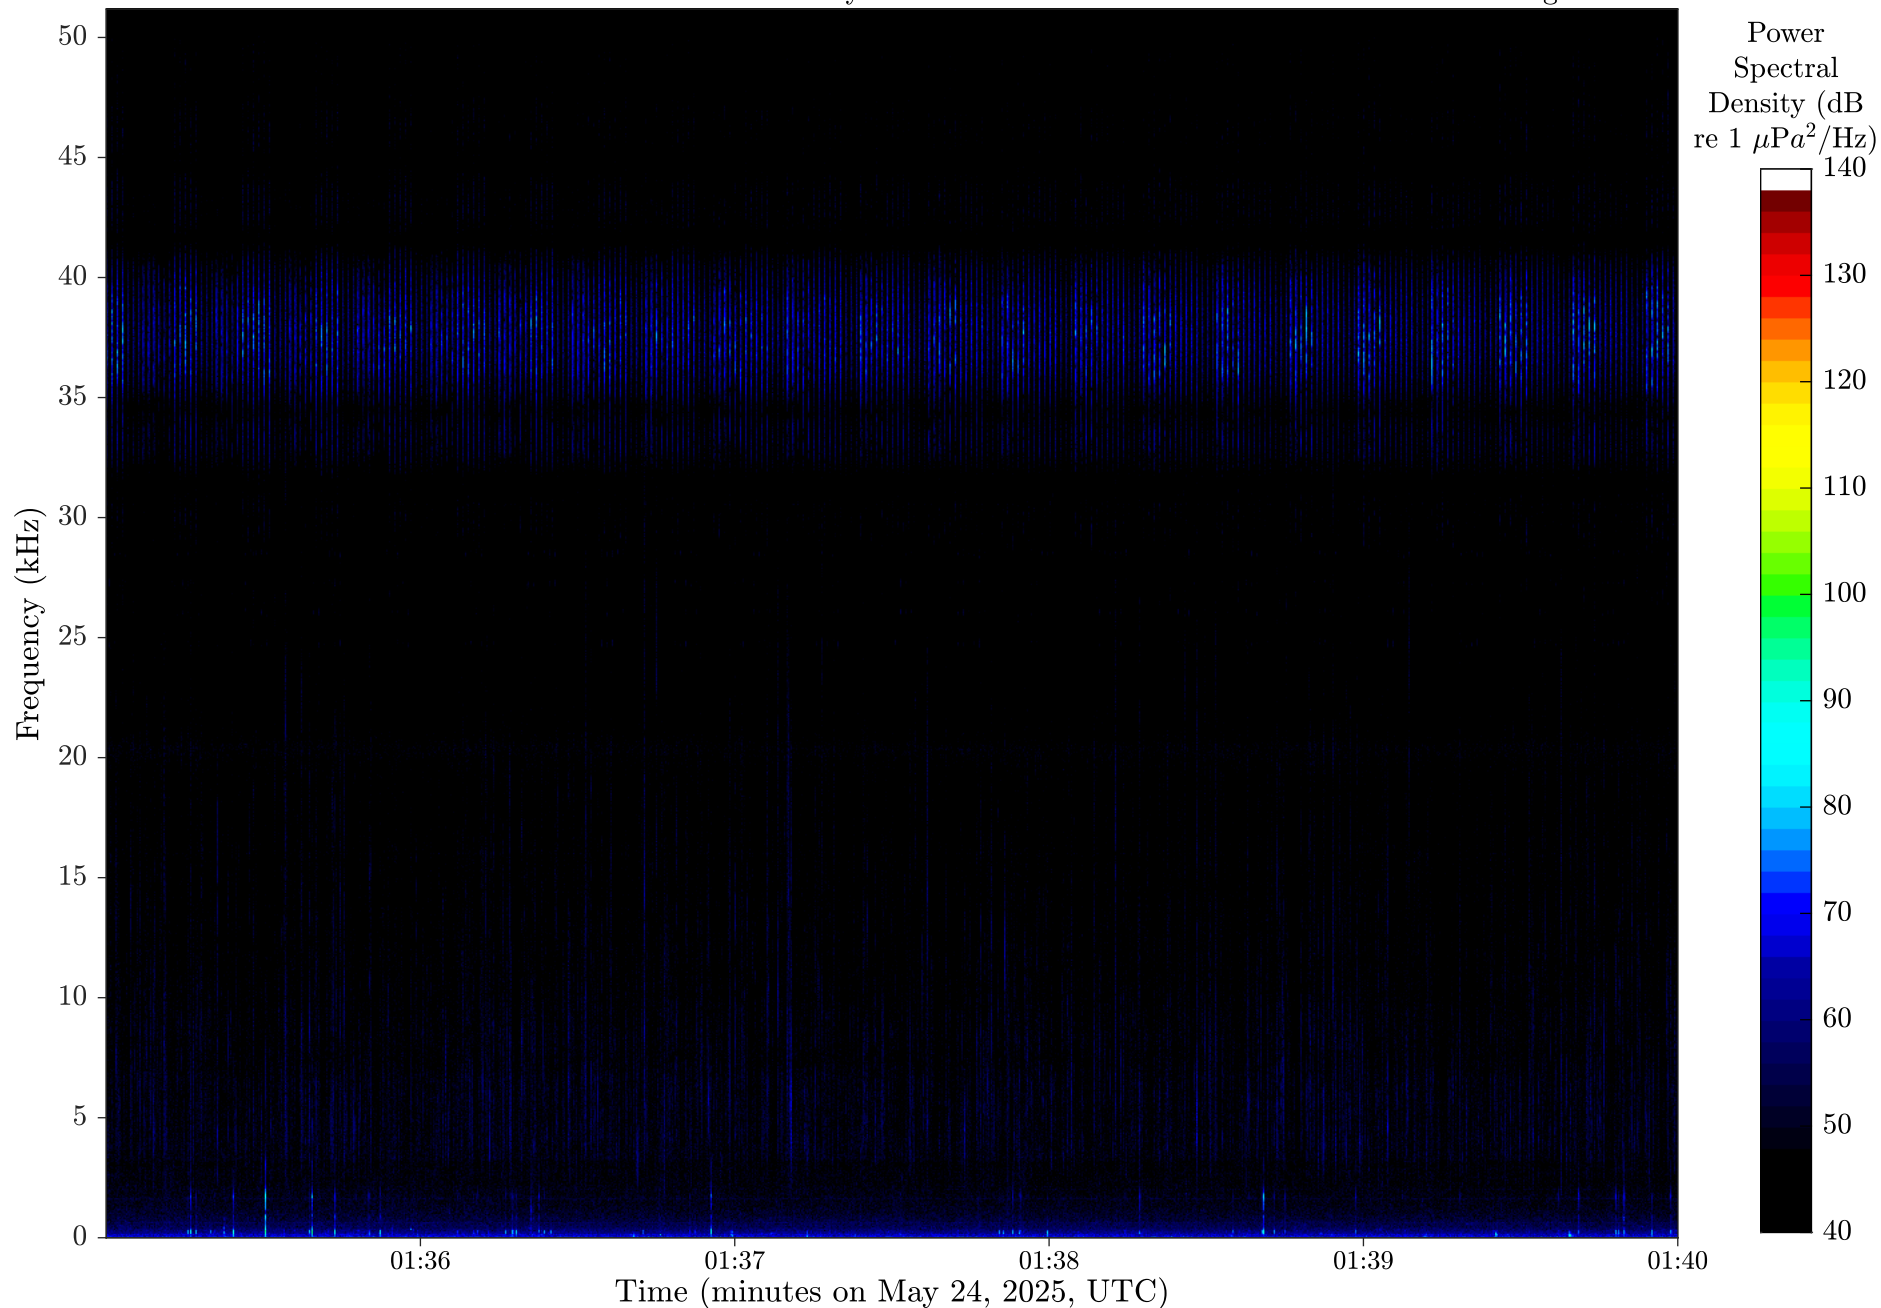


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:33 UTC

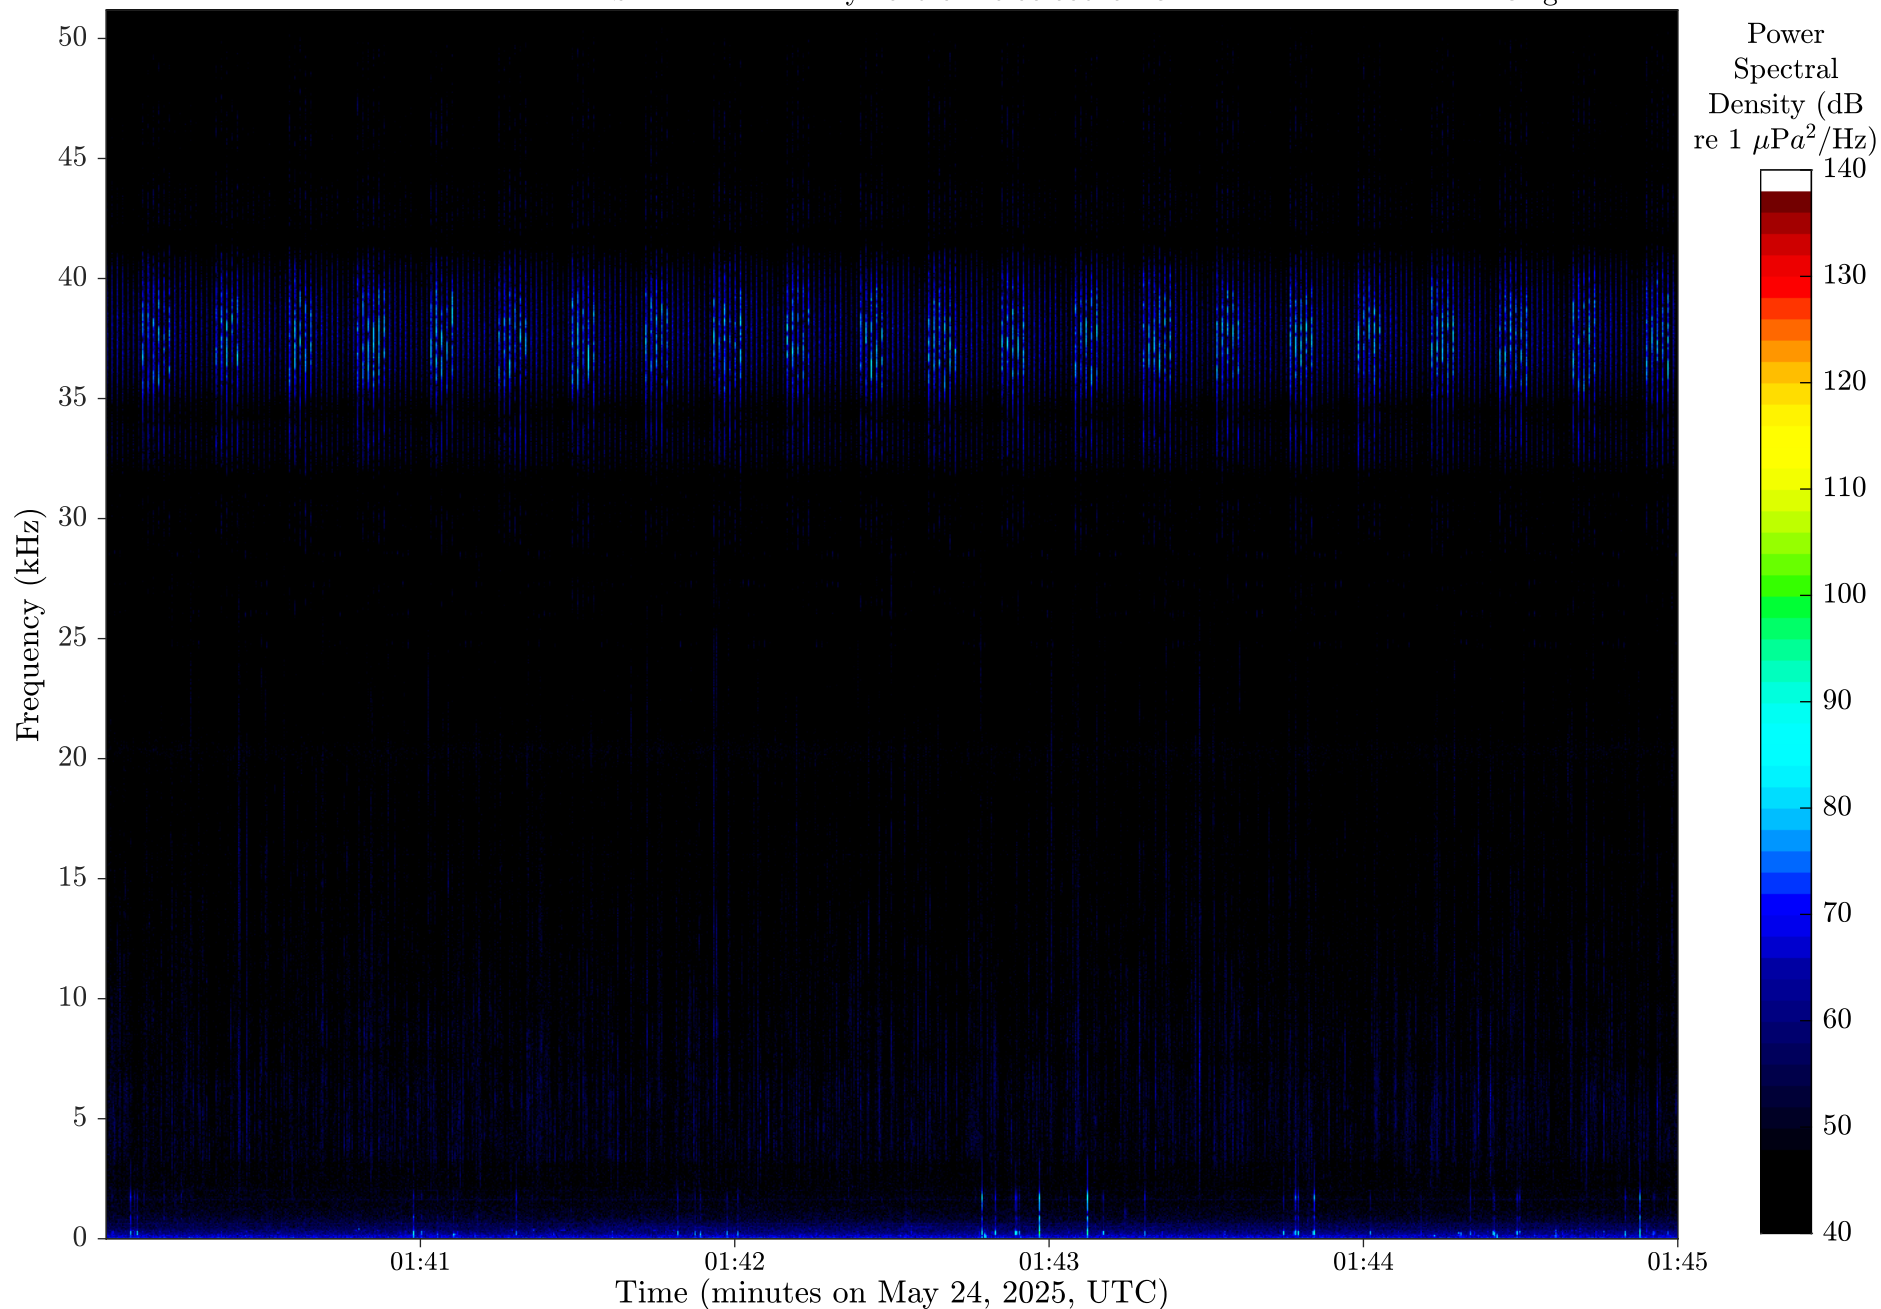


Comments: 34.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:21:42 UTC

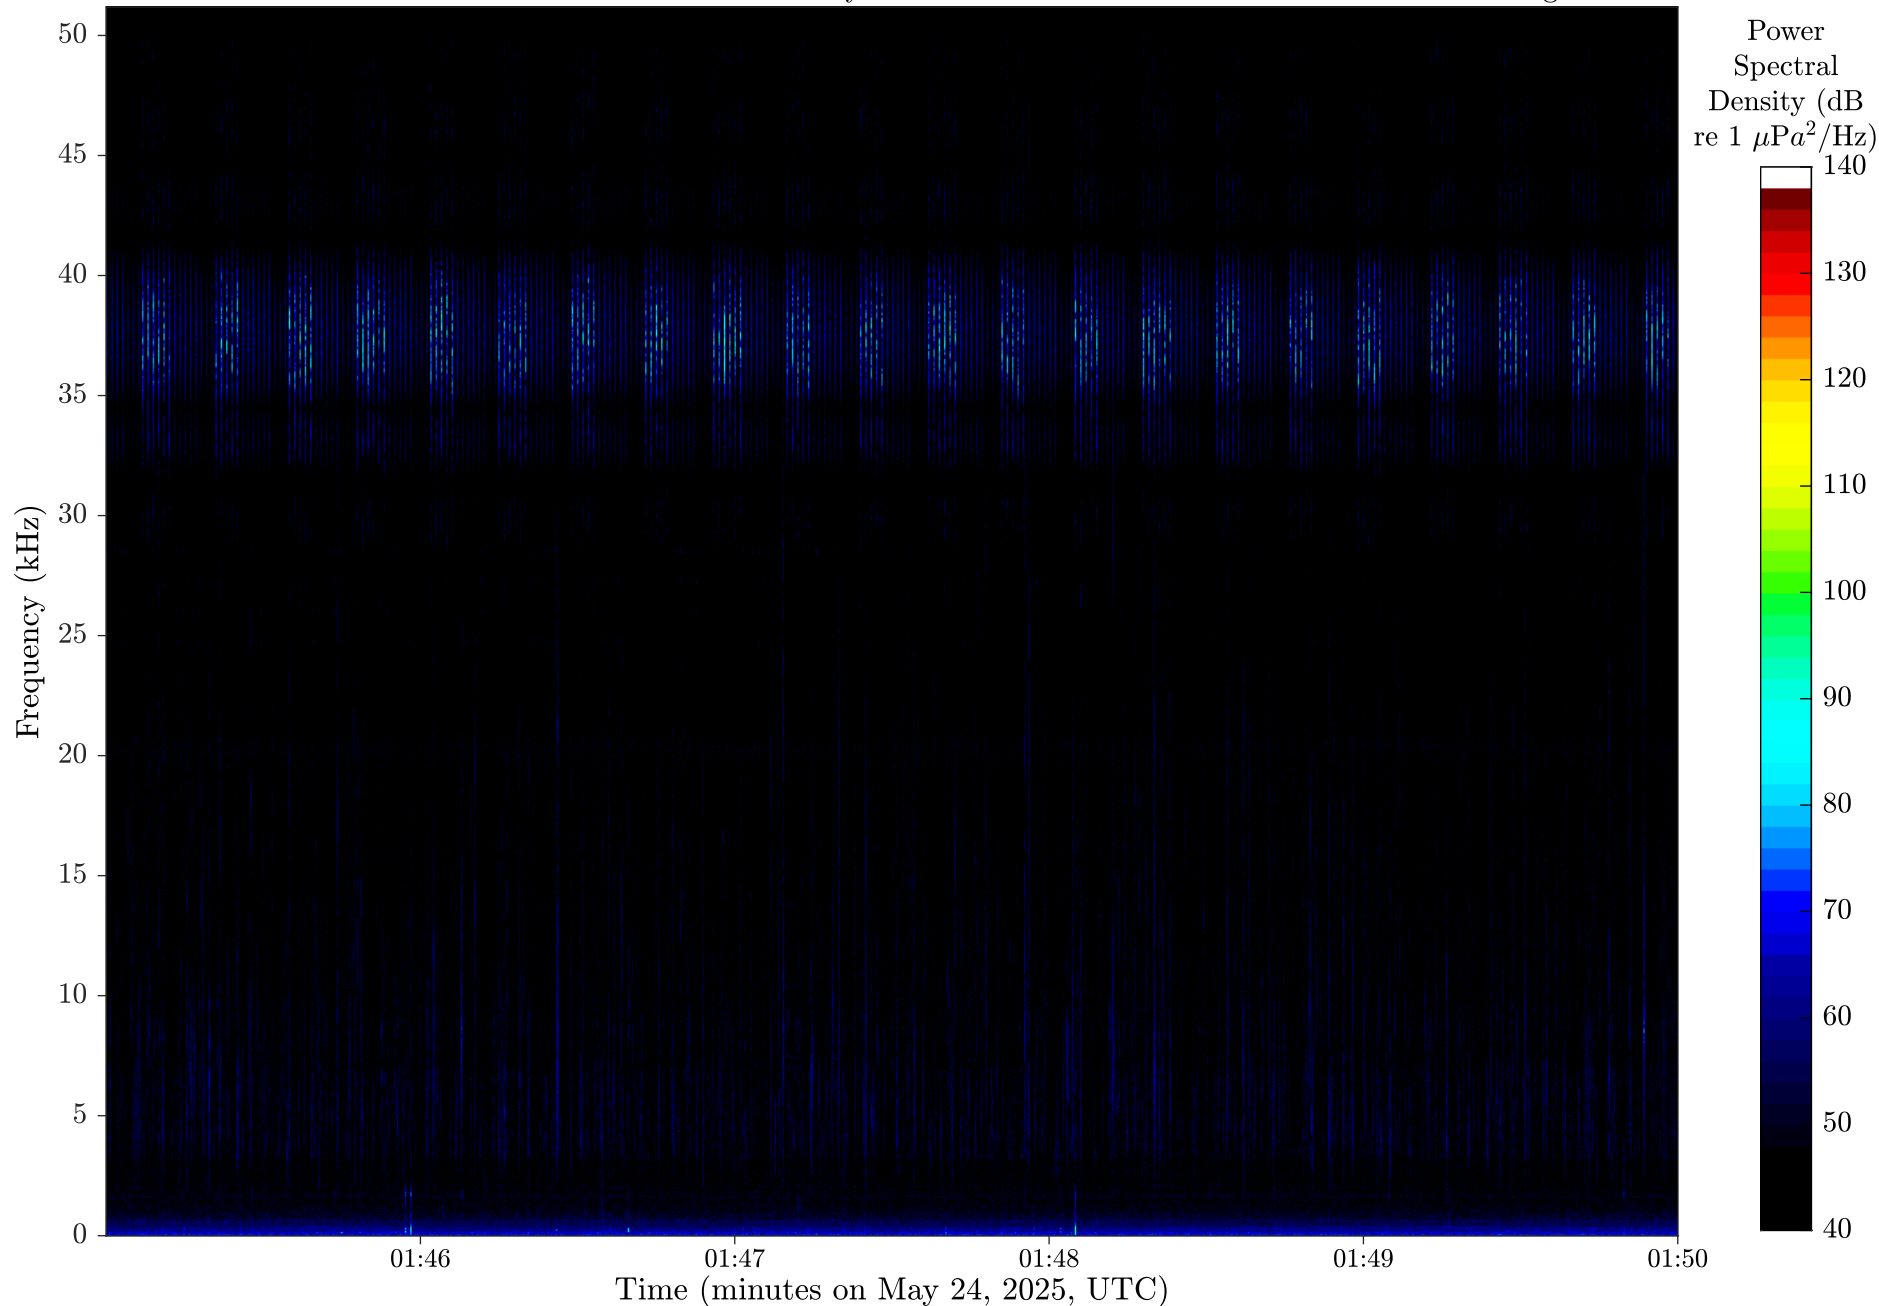


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:21:50 UTC

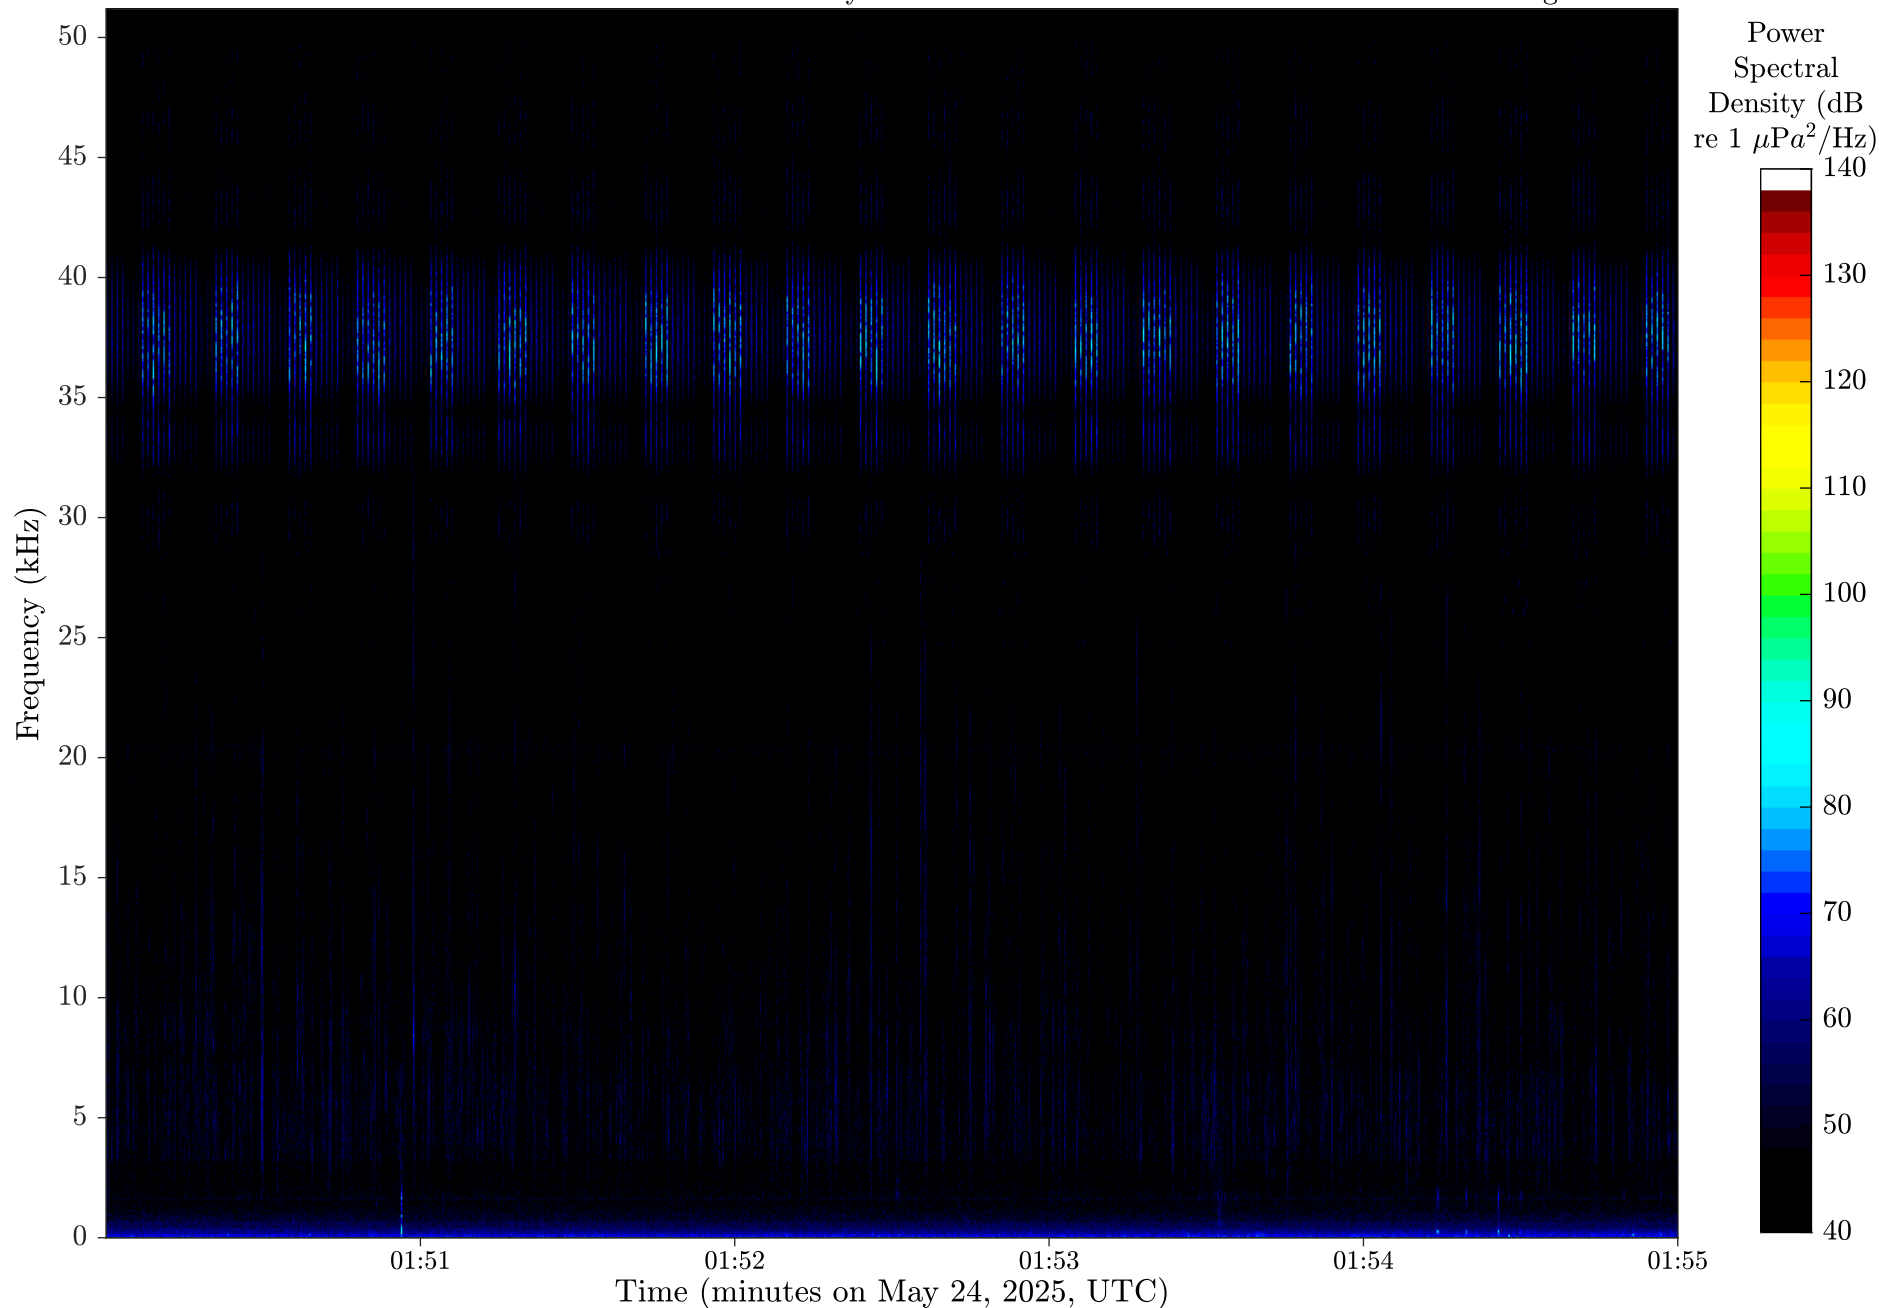


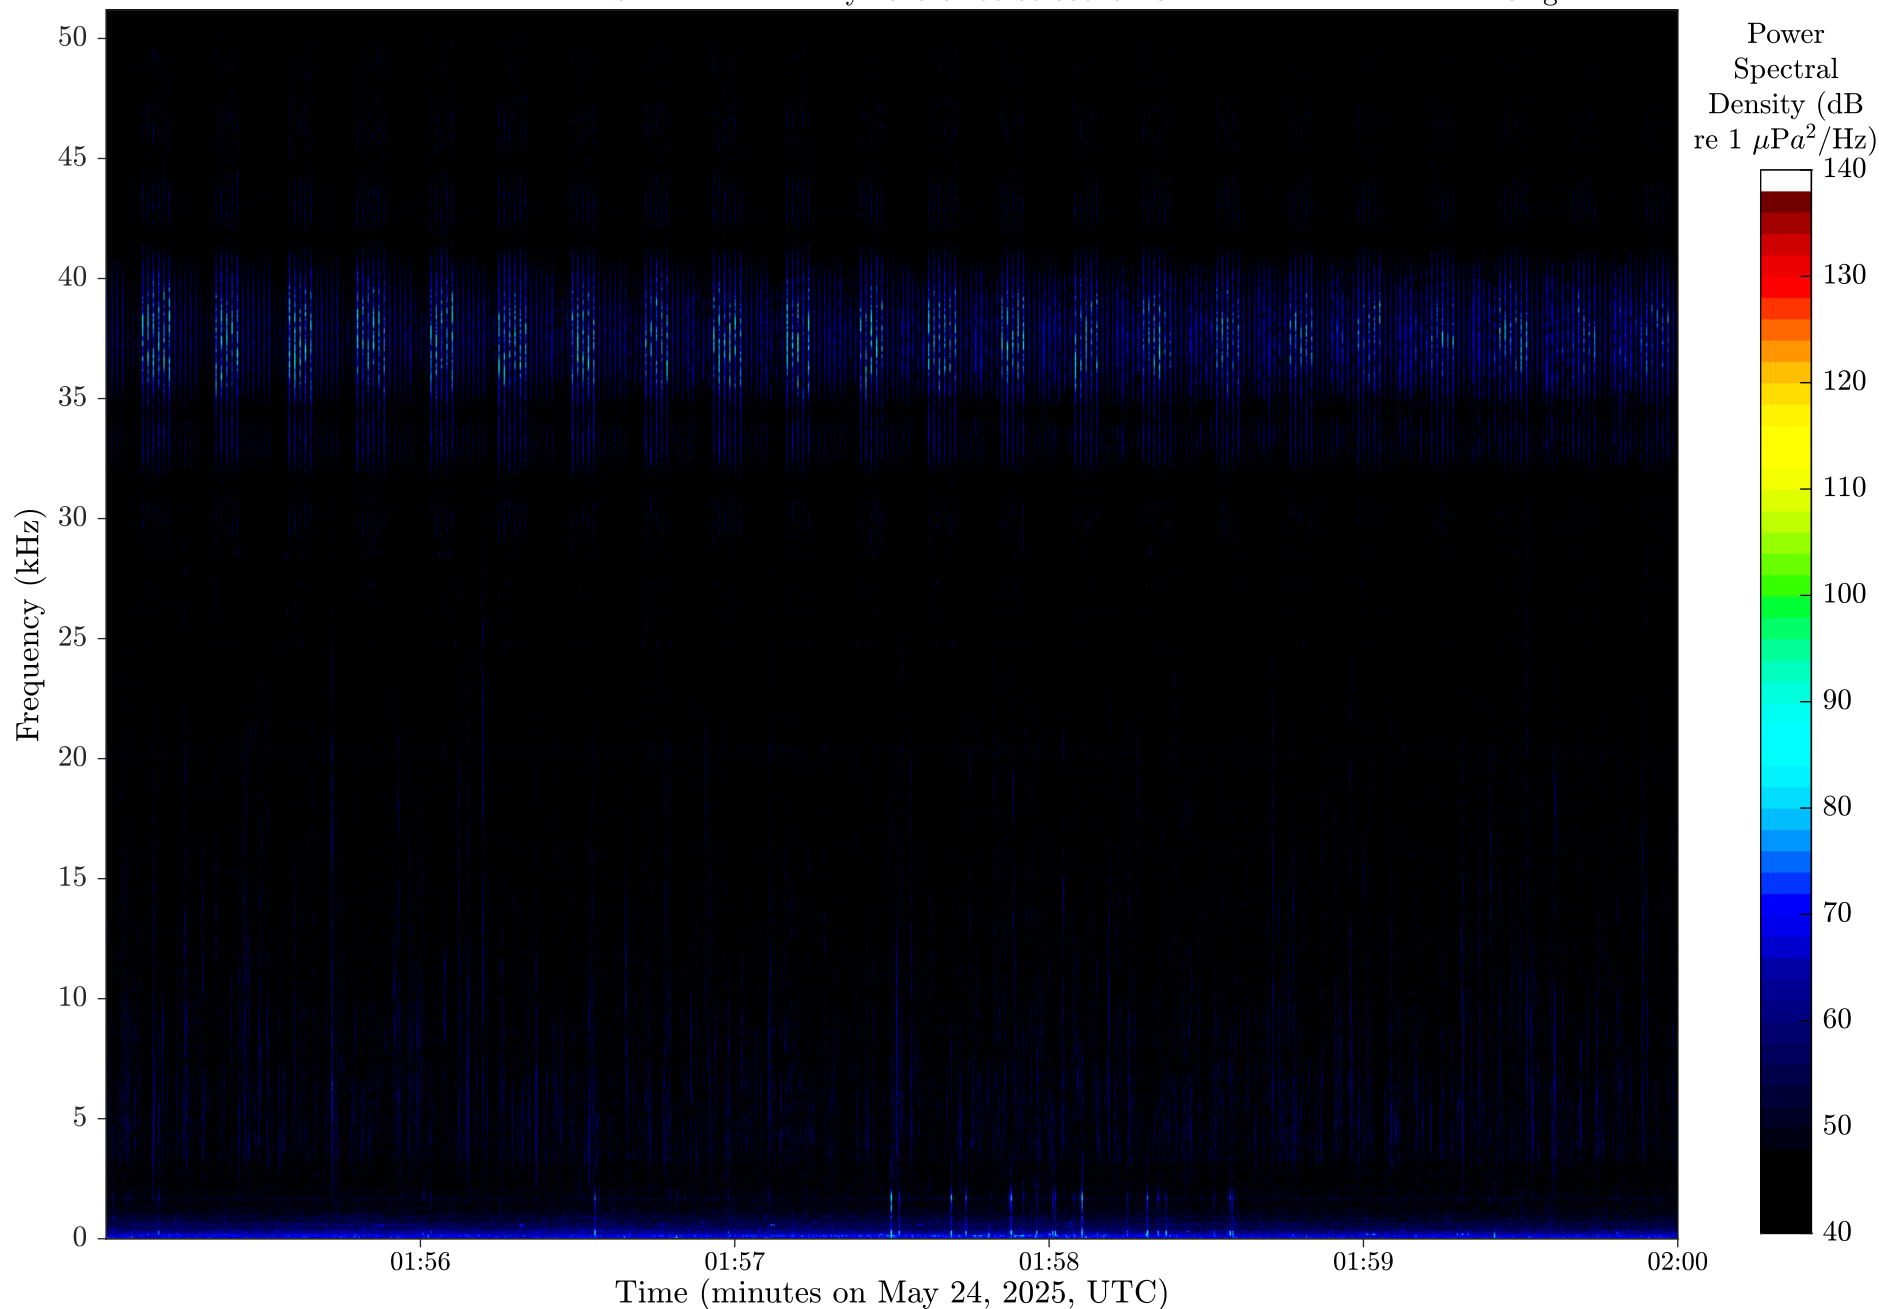

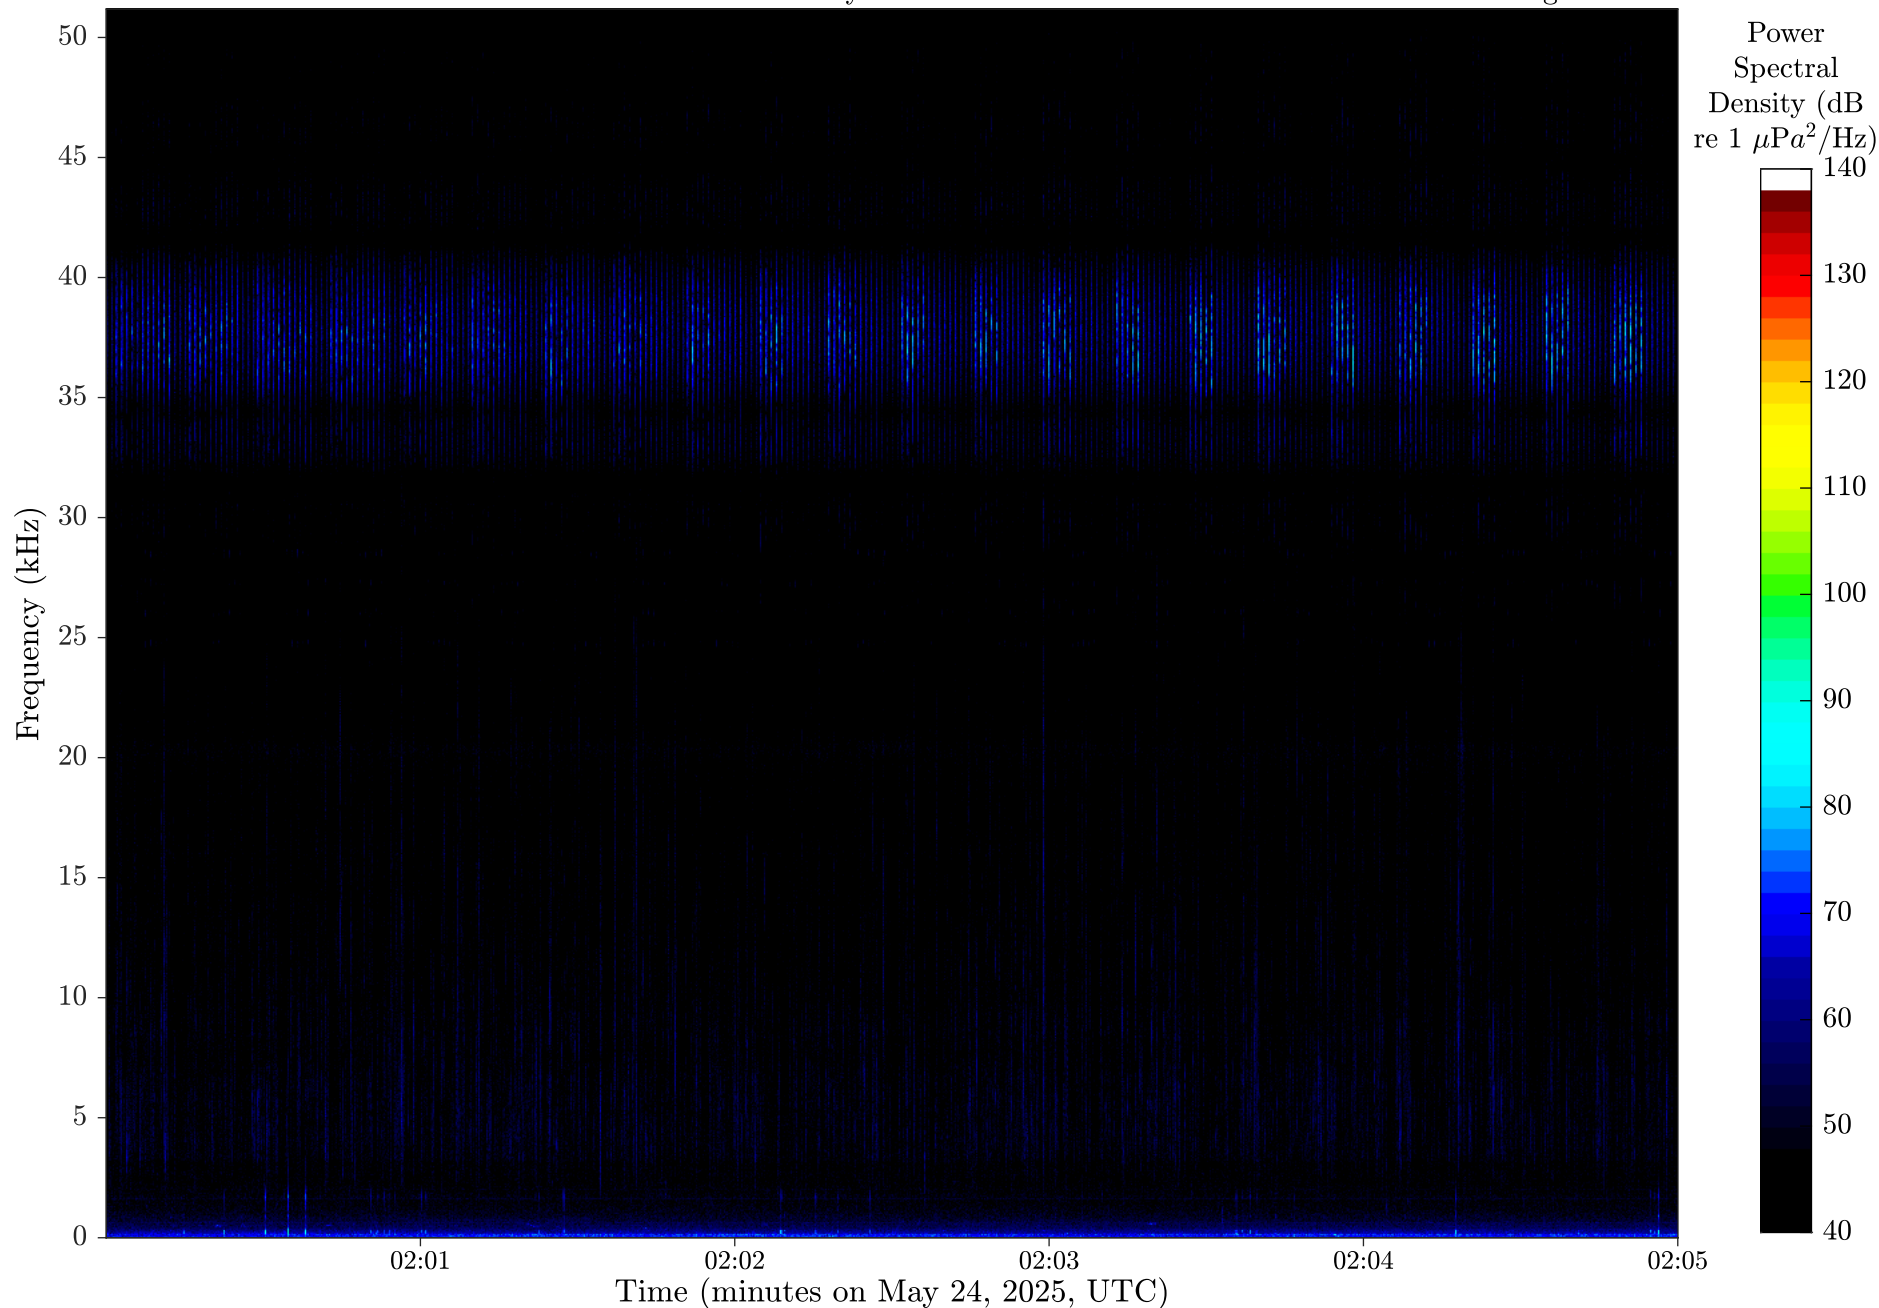


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:17 UTC

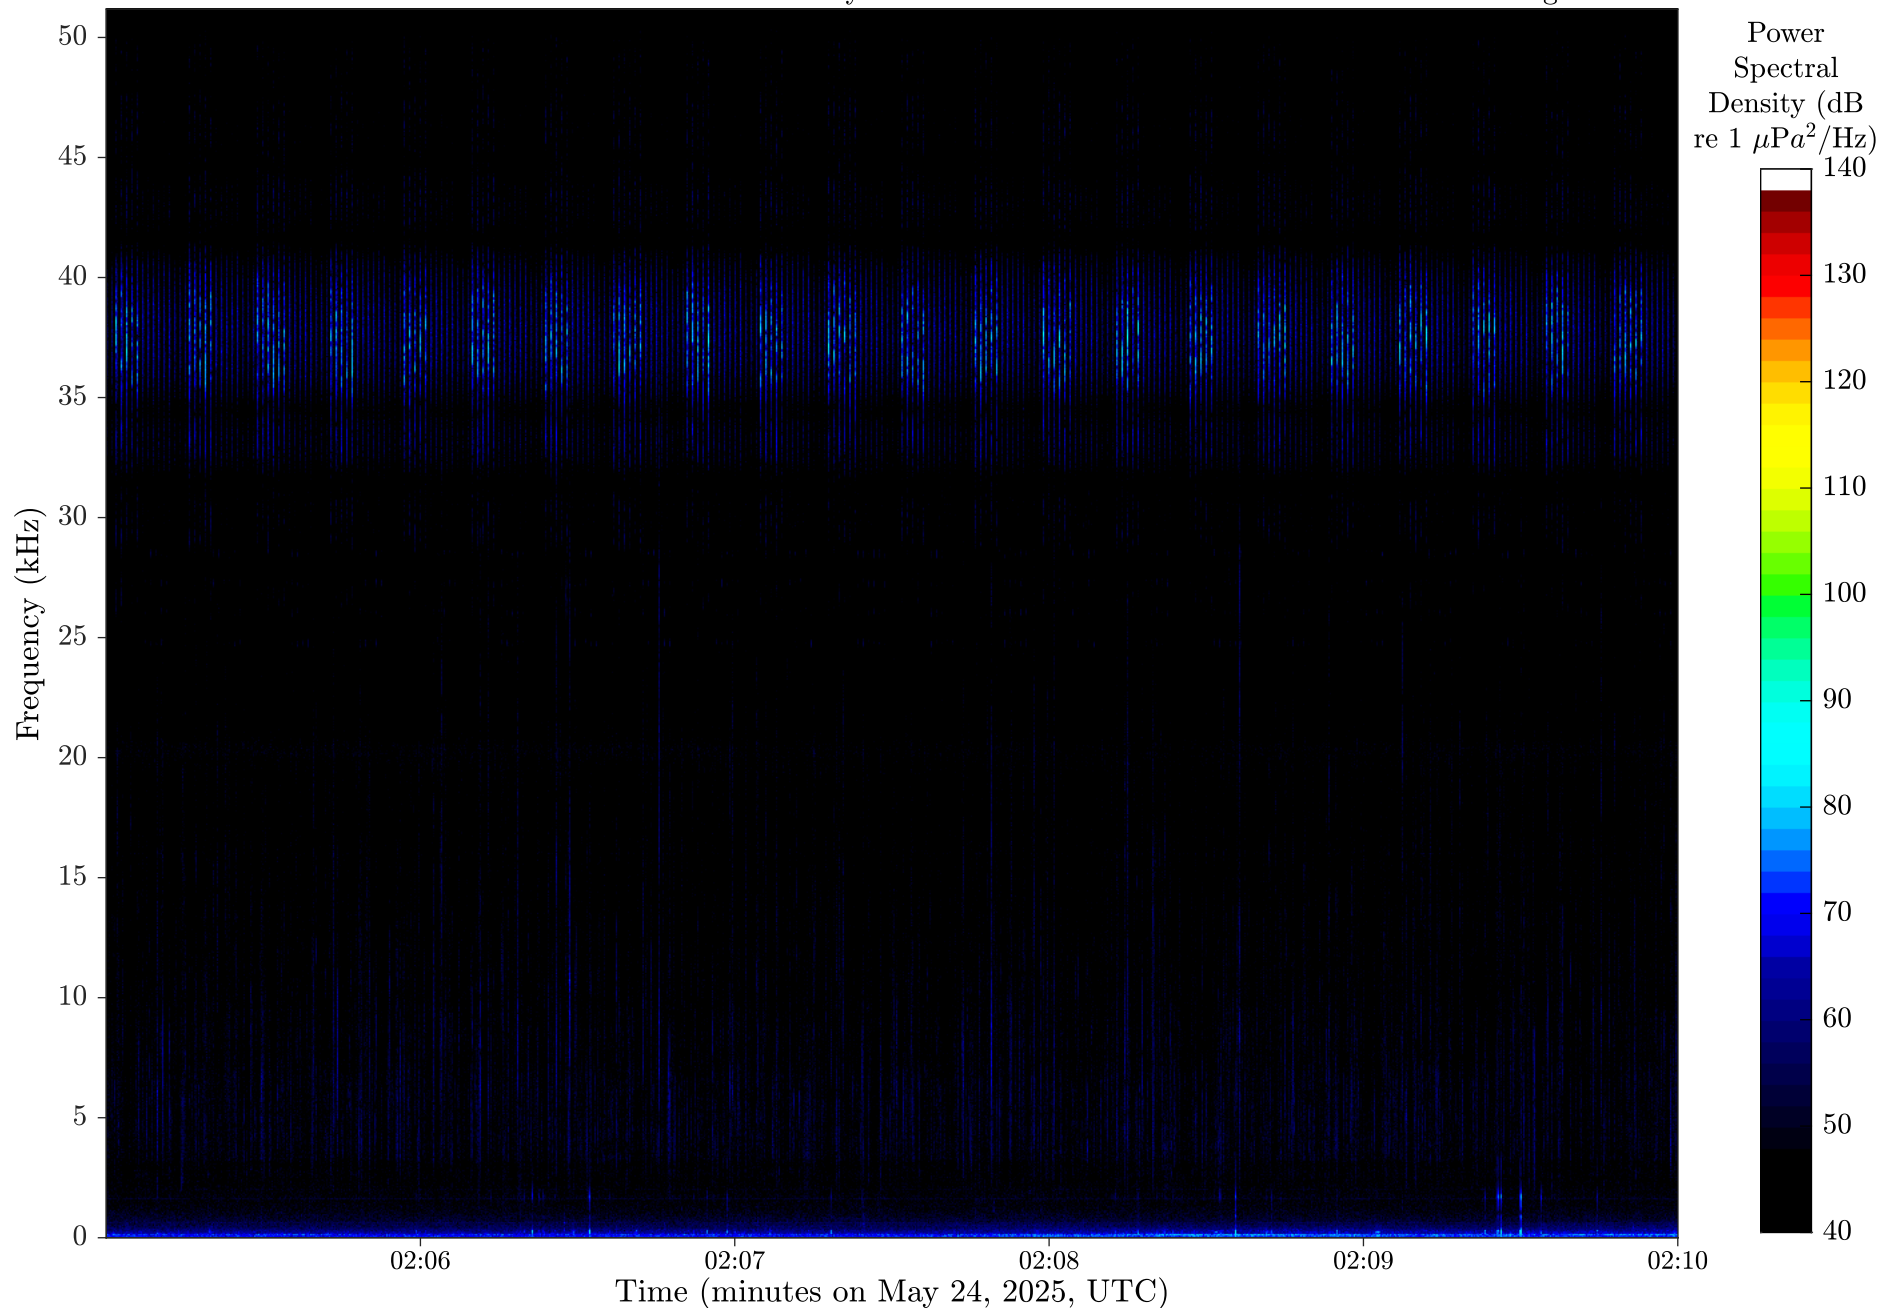


Comments: 35.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:25 UTC

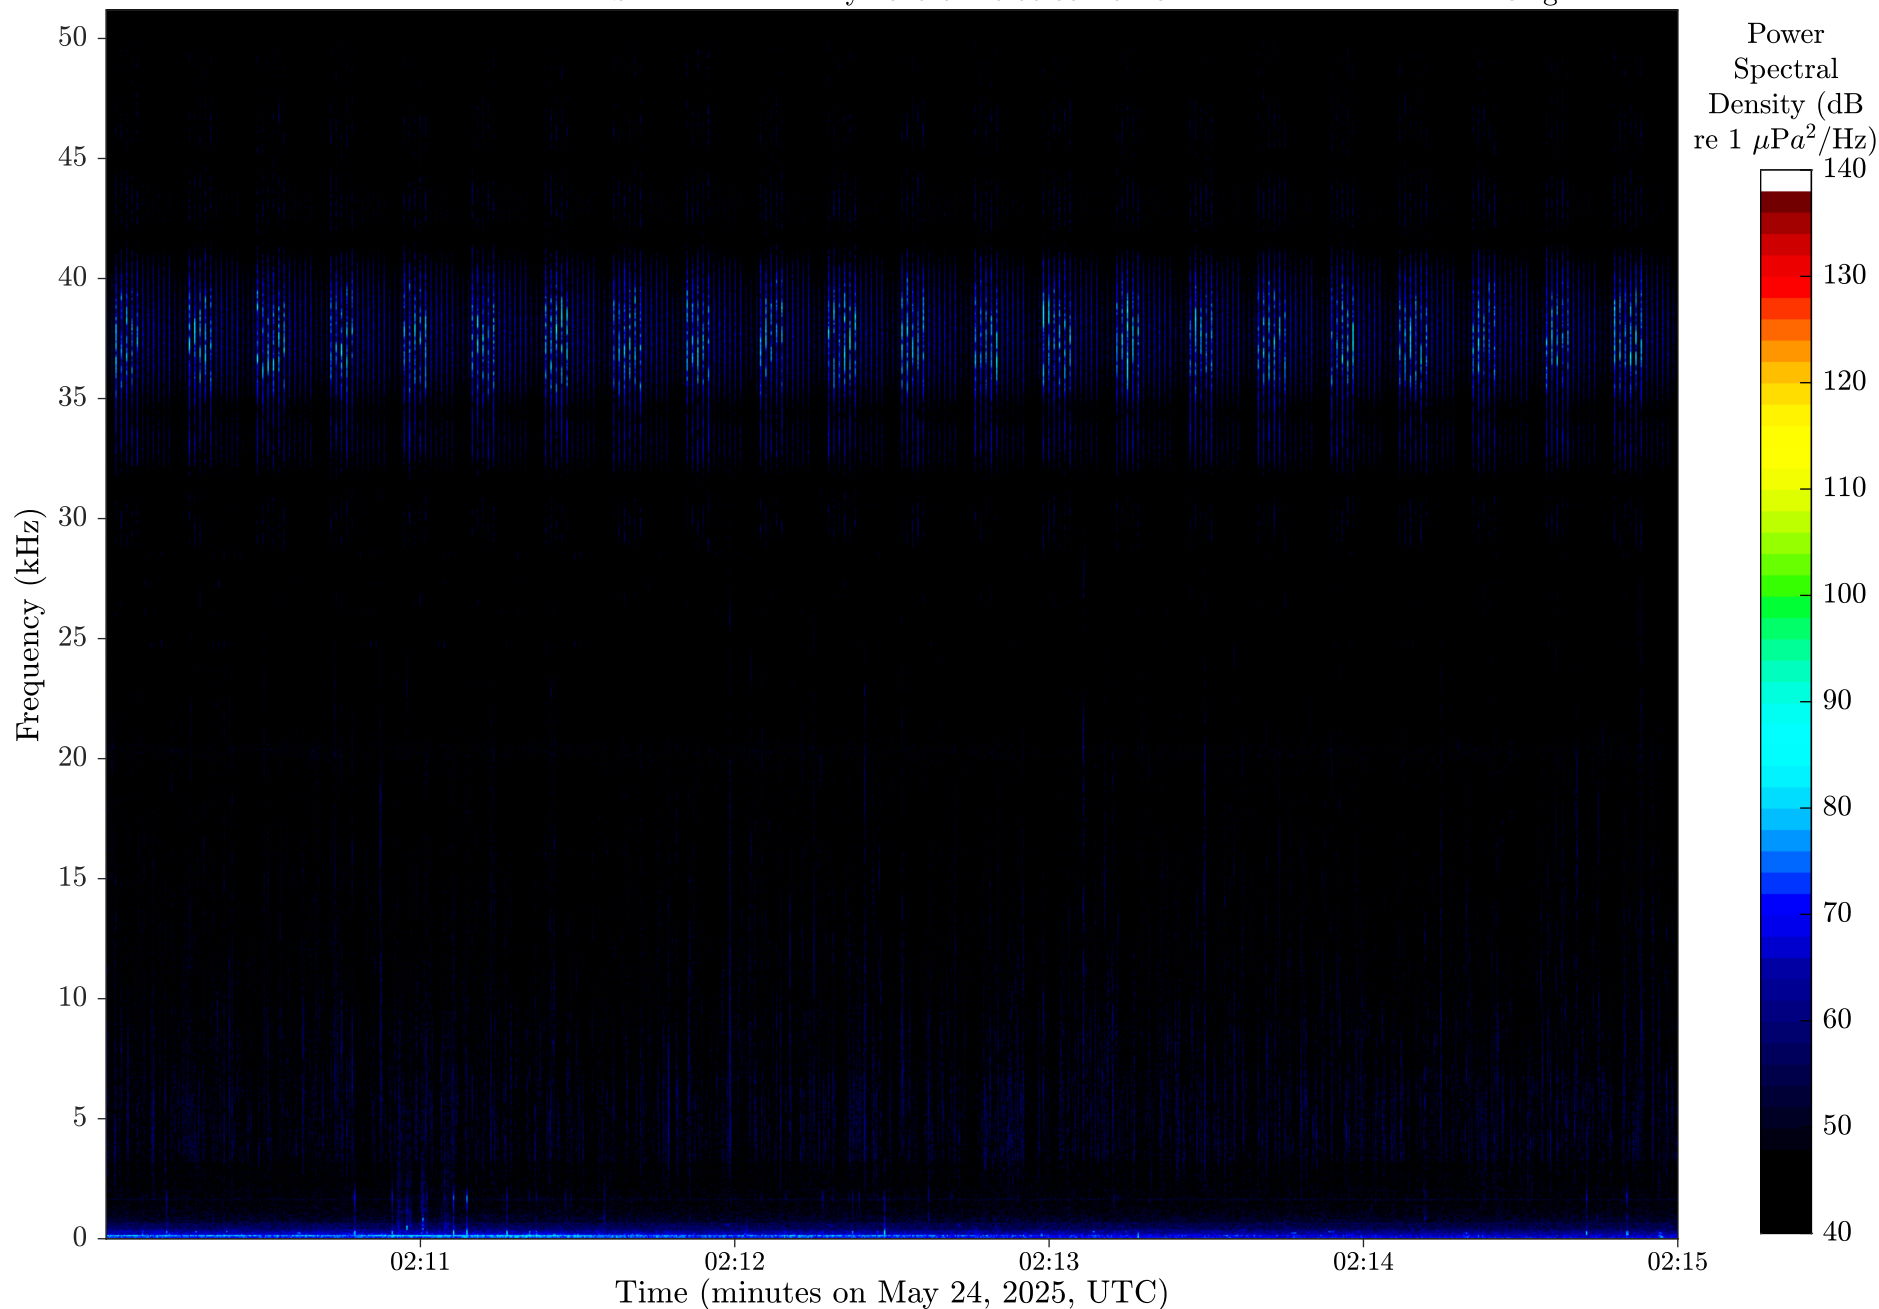


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:34 UTC

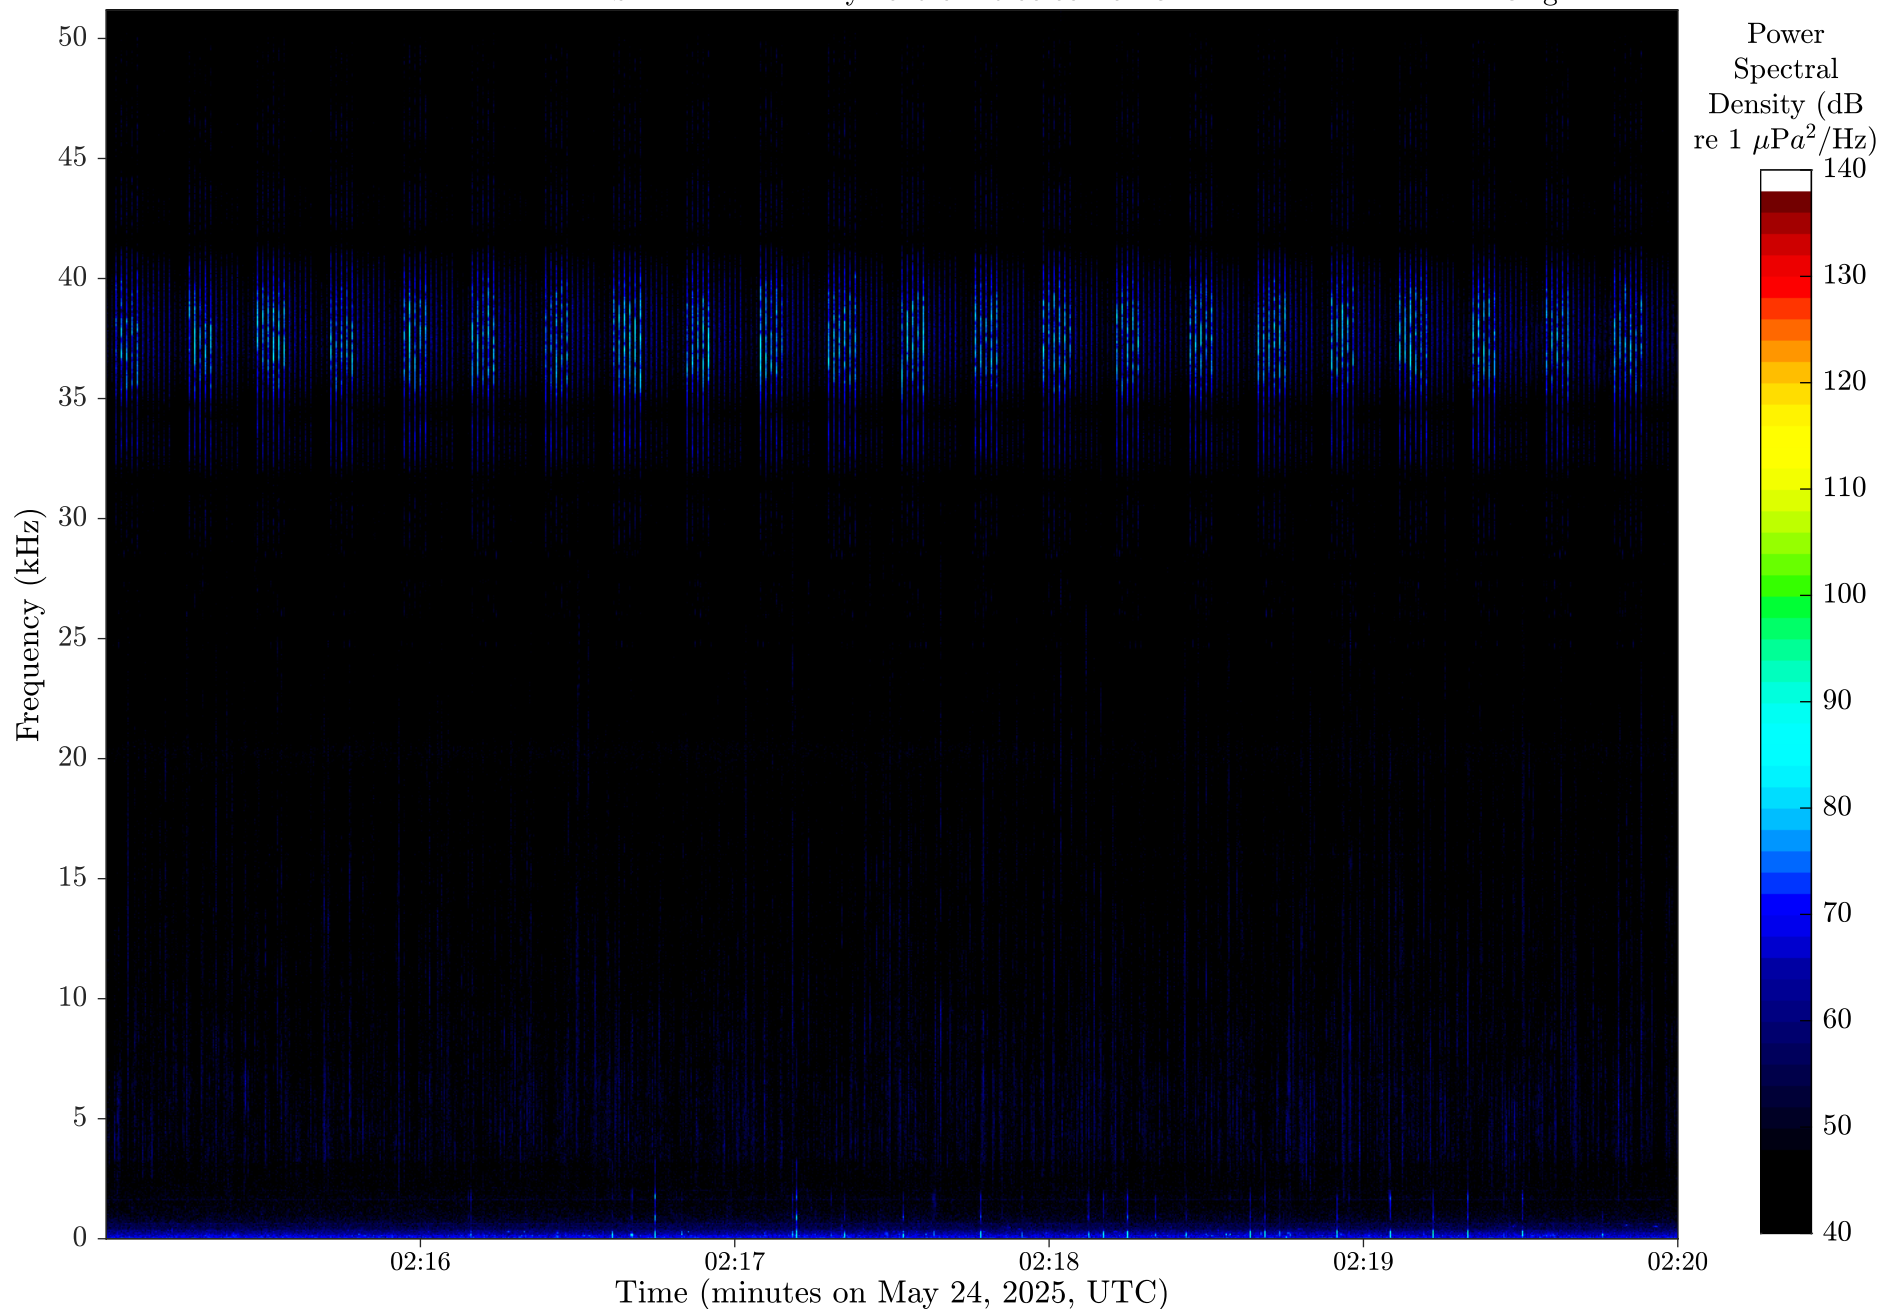


Comments: 35.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:42 UTC

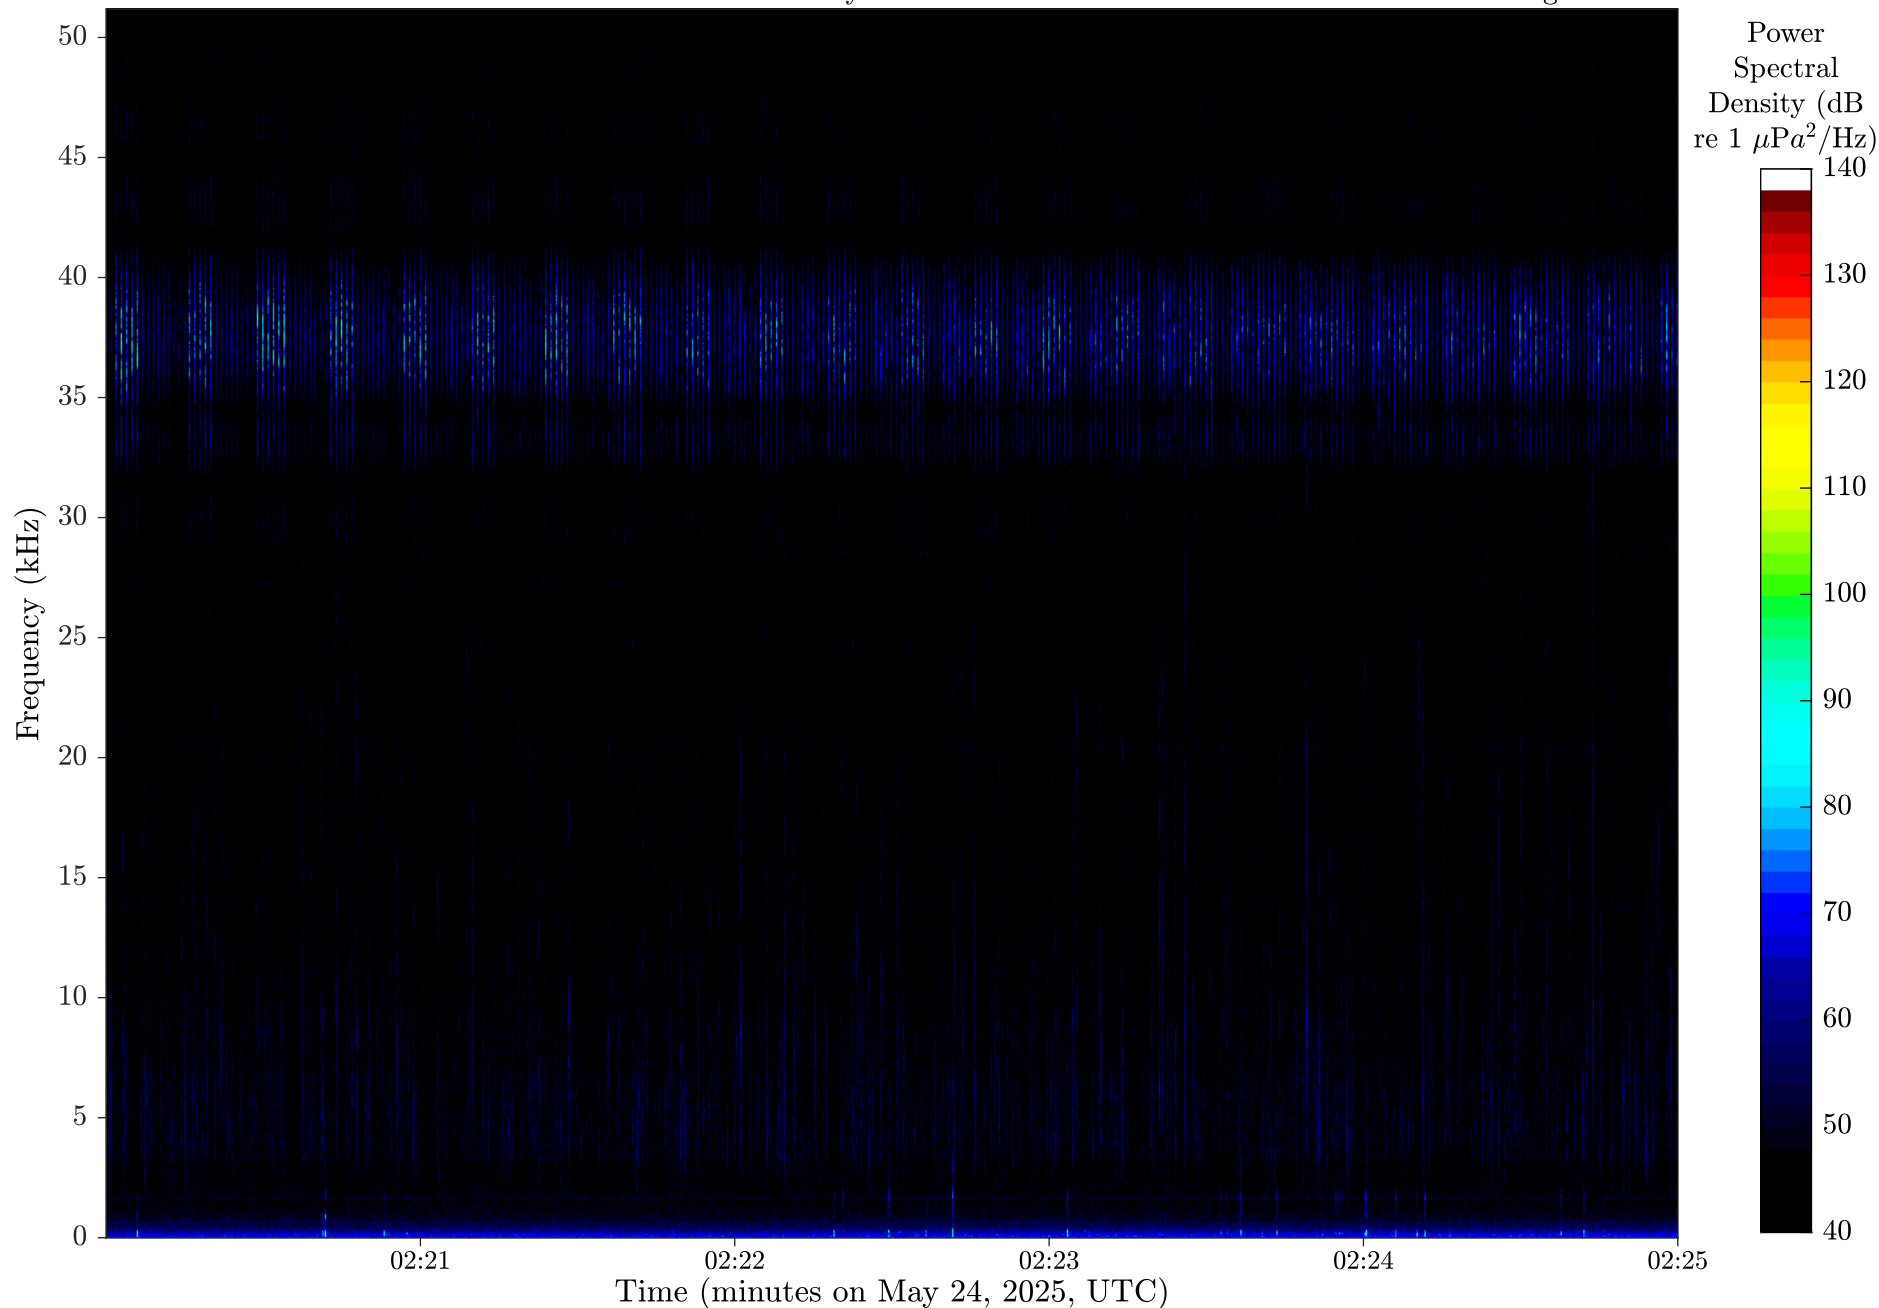


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:22:52 UTC

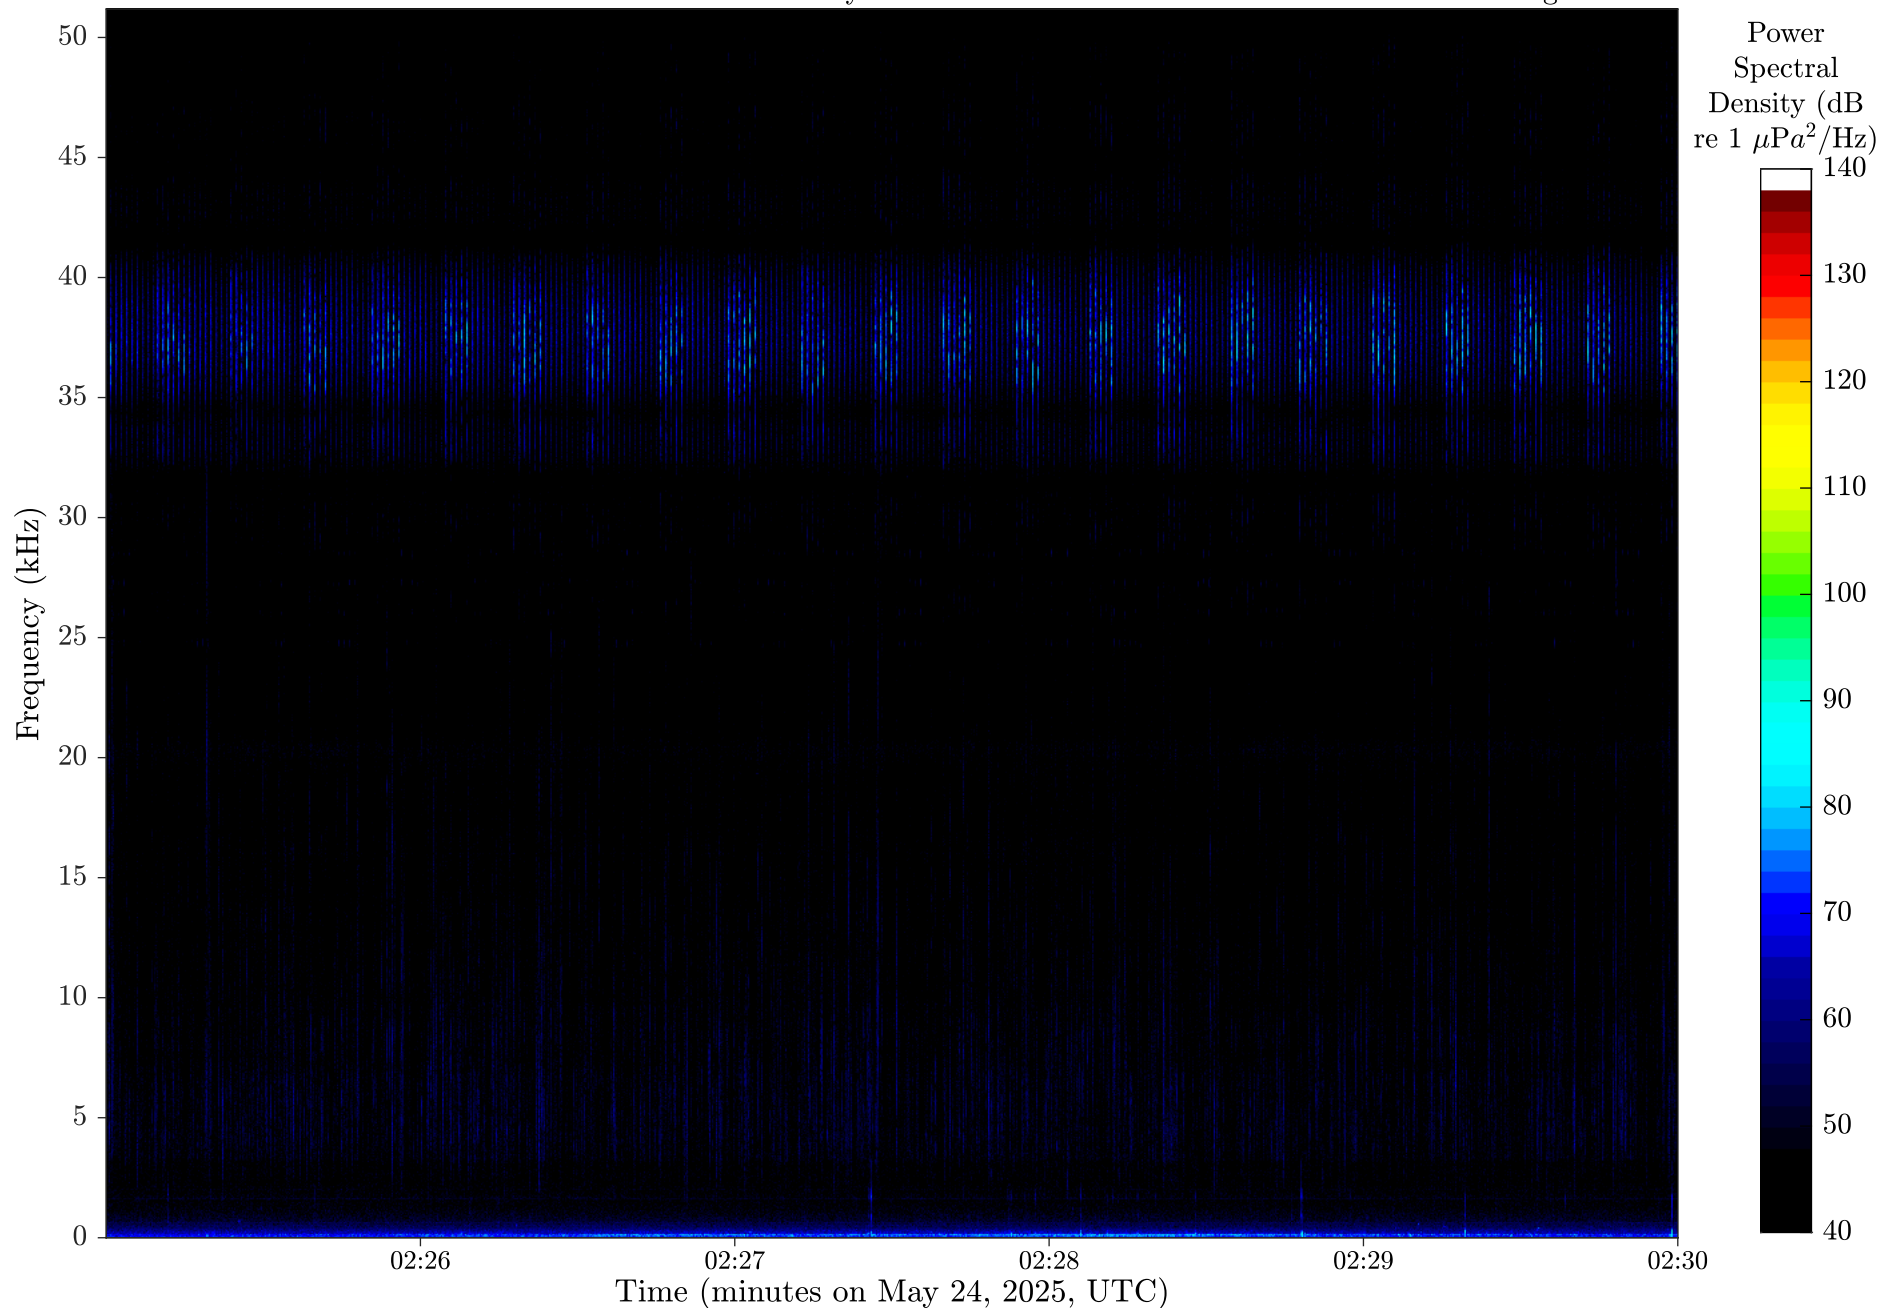


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:01 UTC

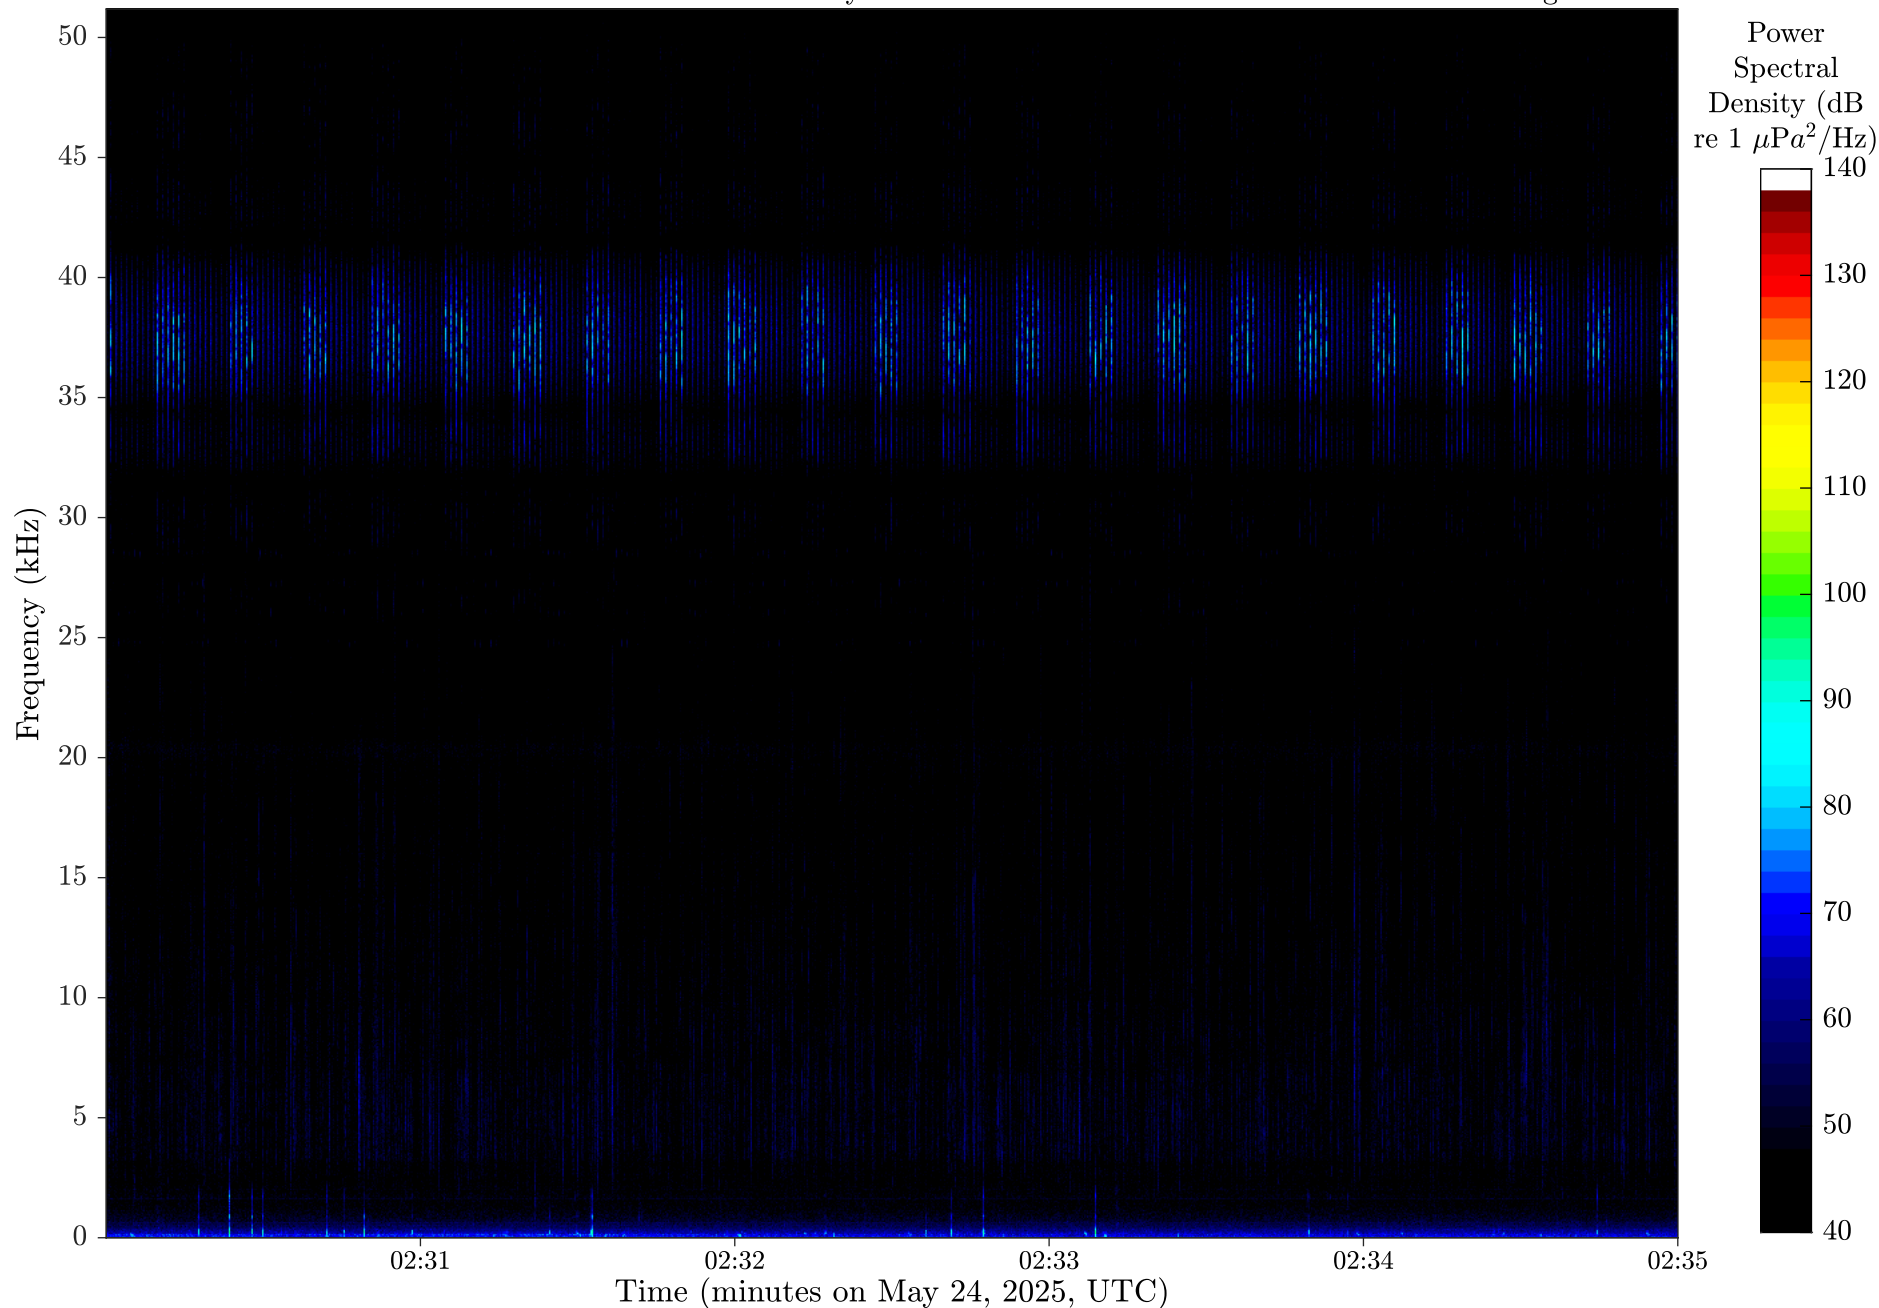


Comments: 35.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:23:09 UTC

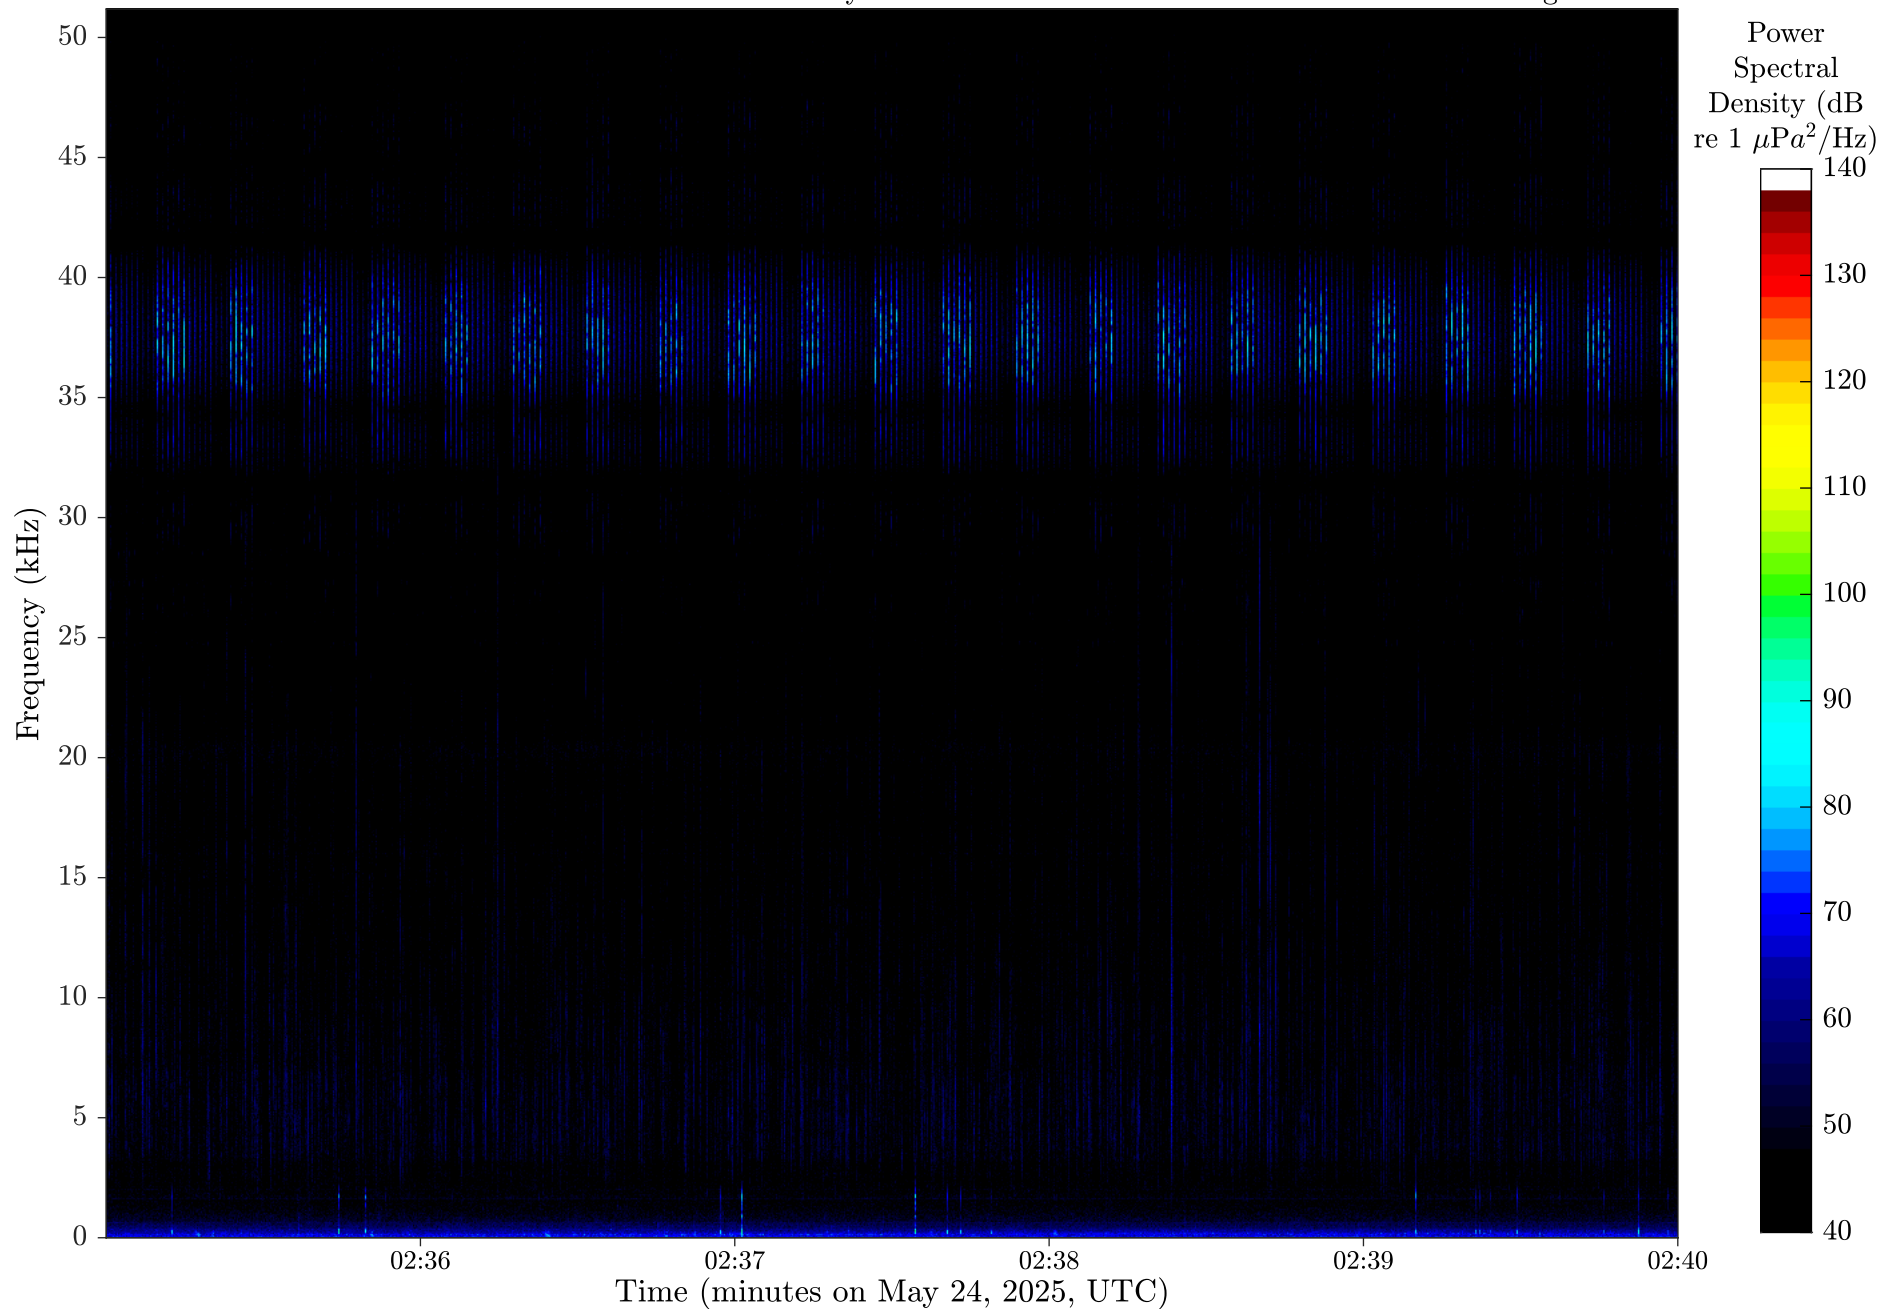

Comments: 36.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:23:18 UTC

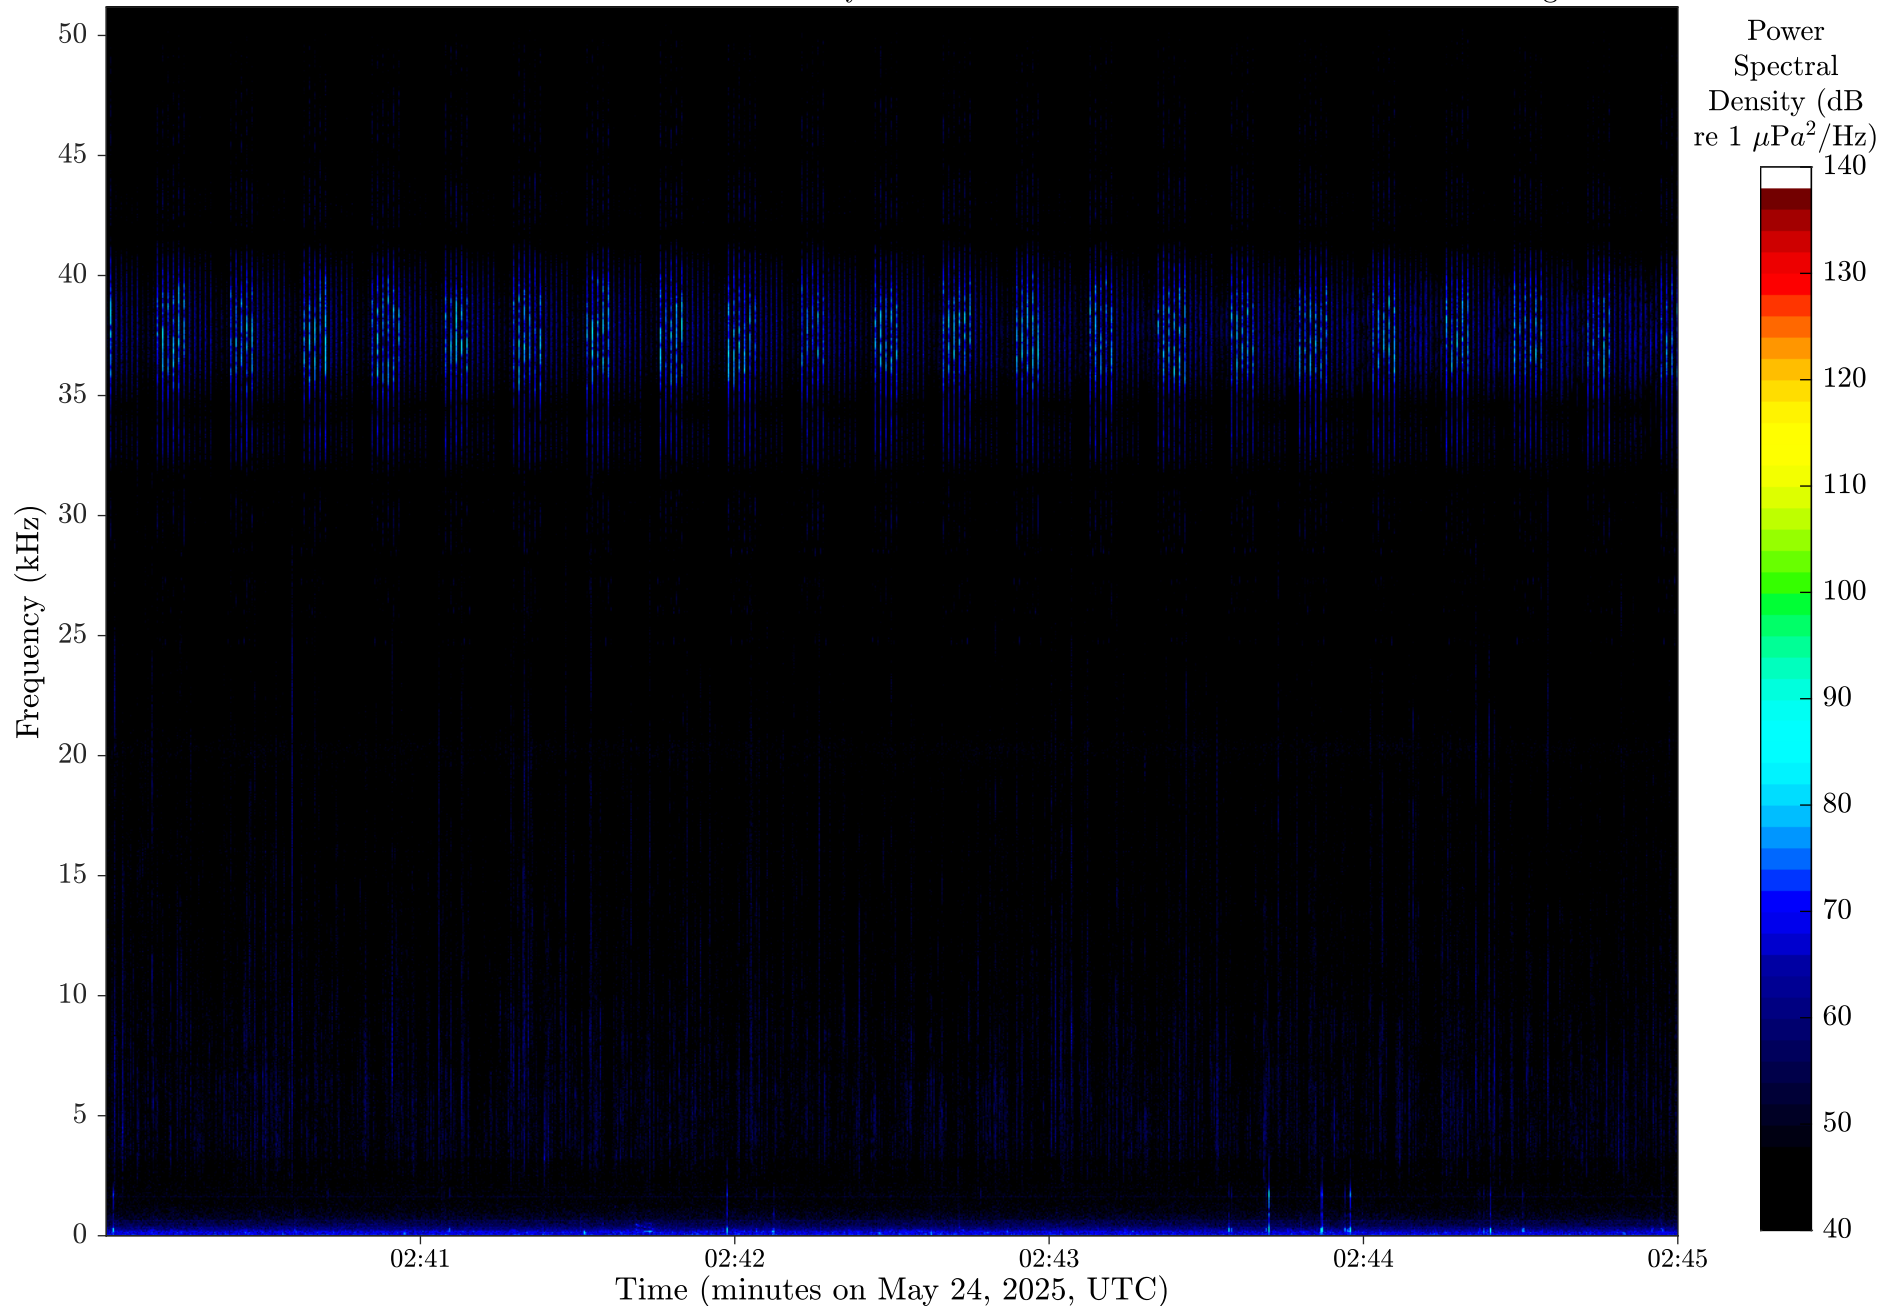

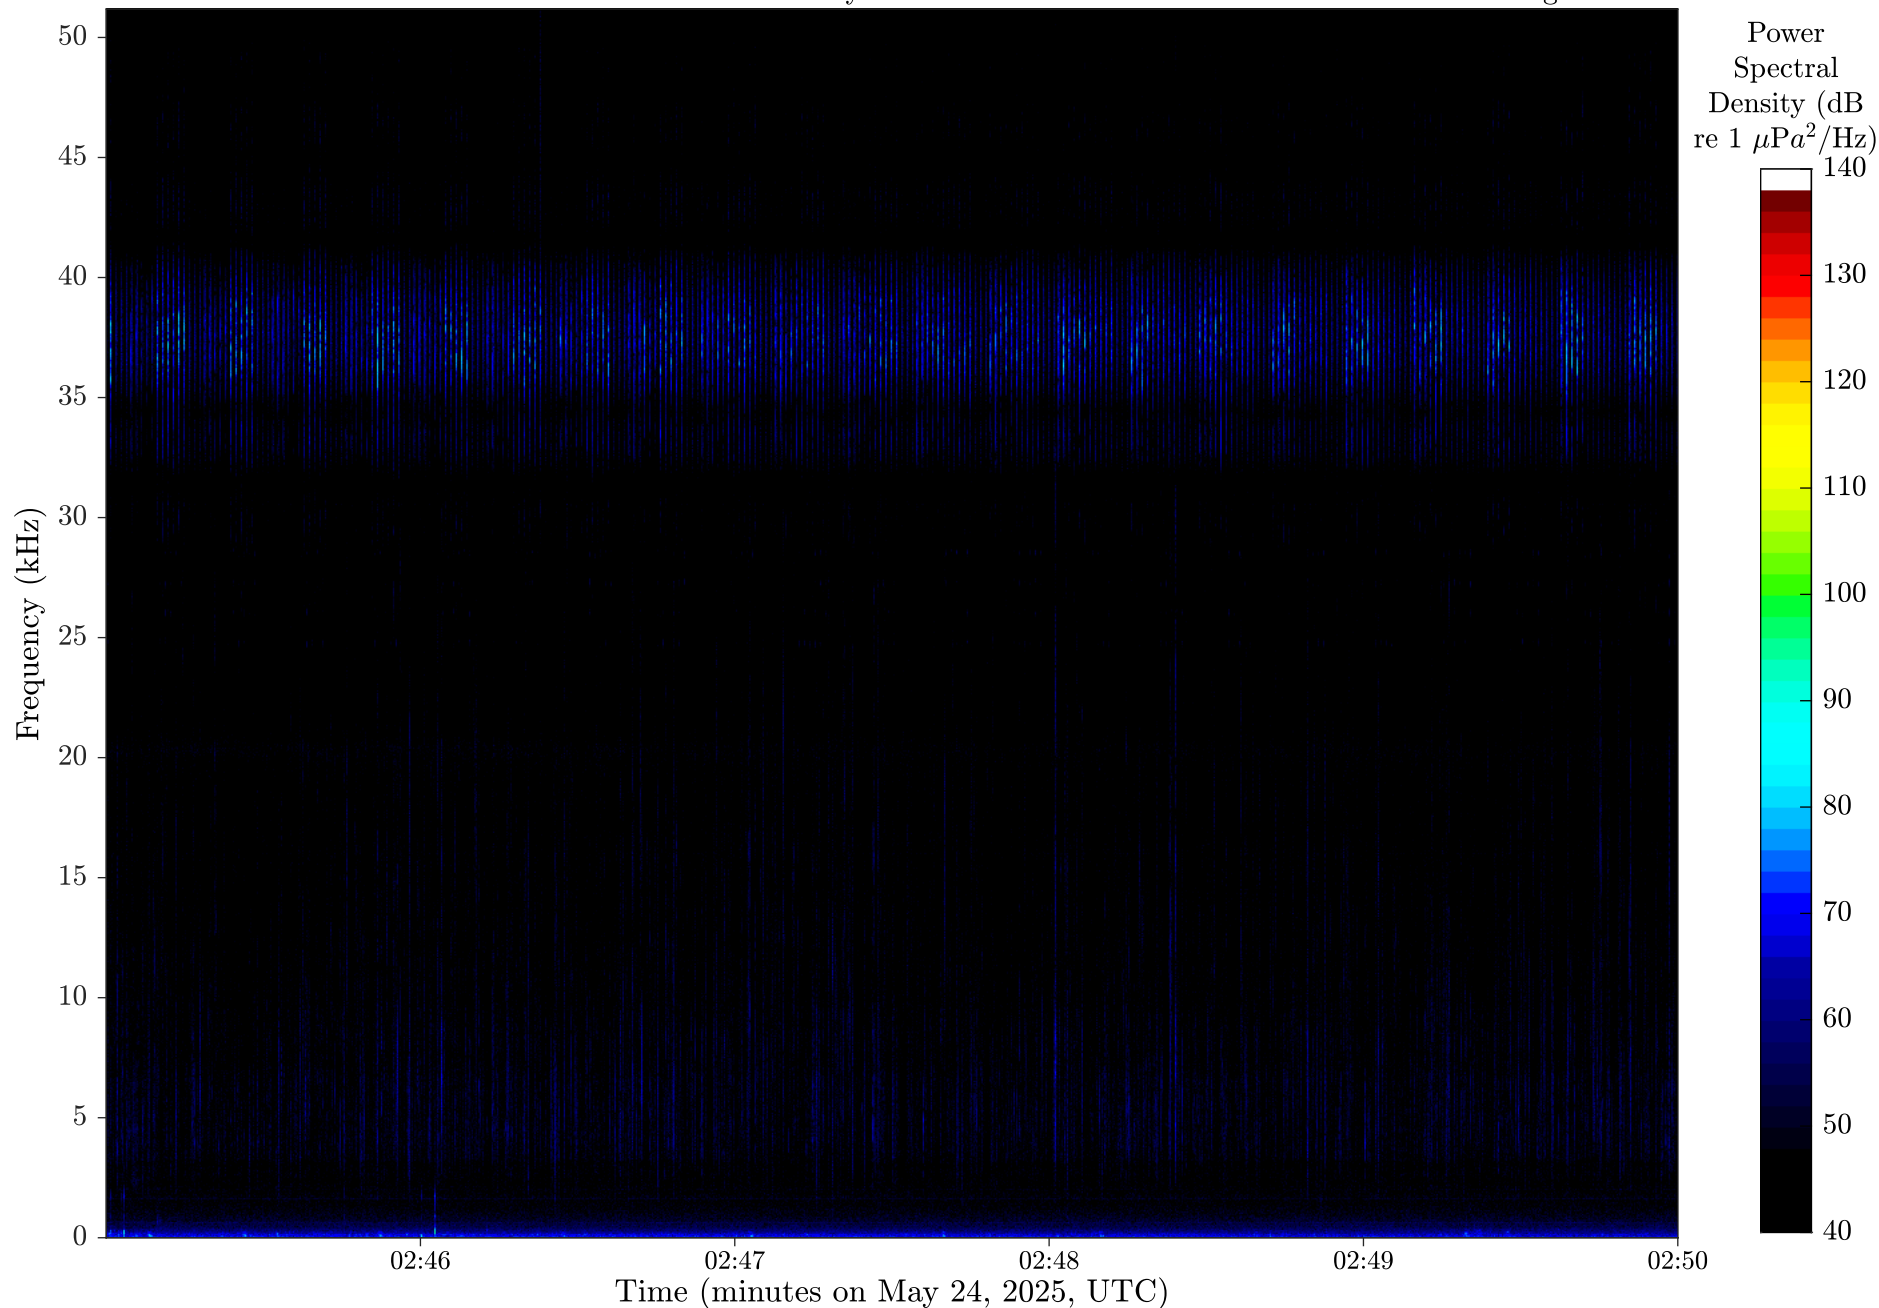


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:23:35 UTC

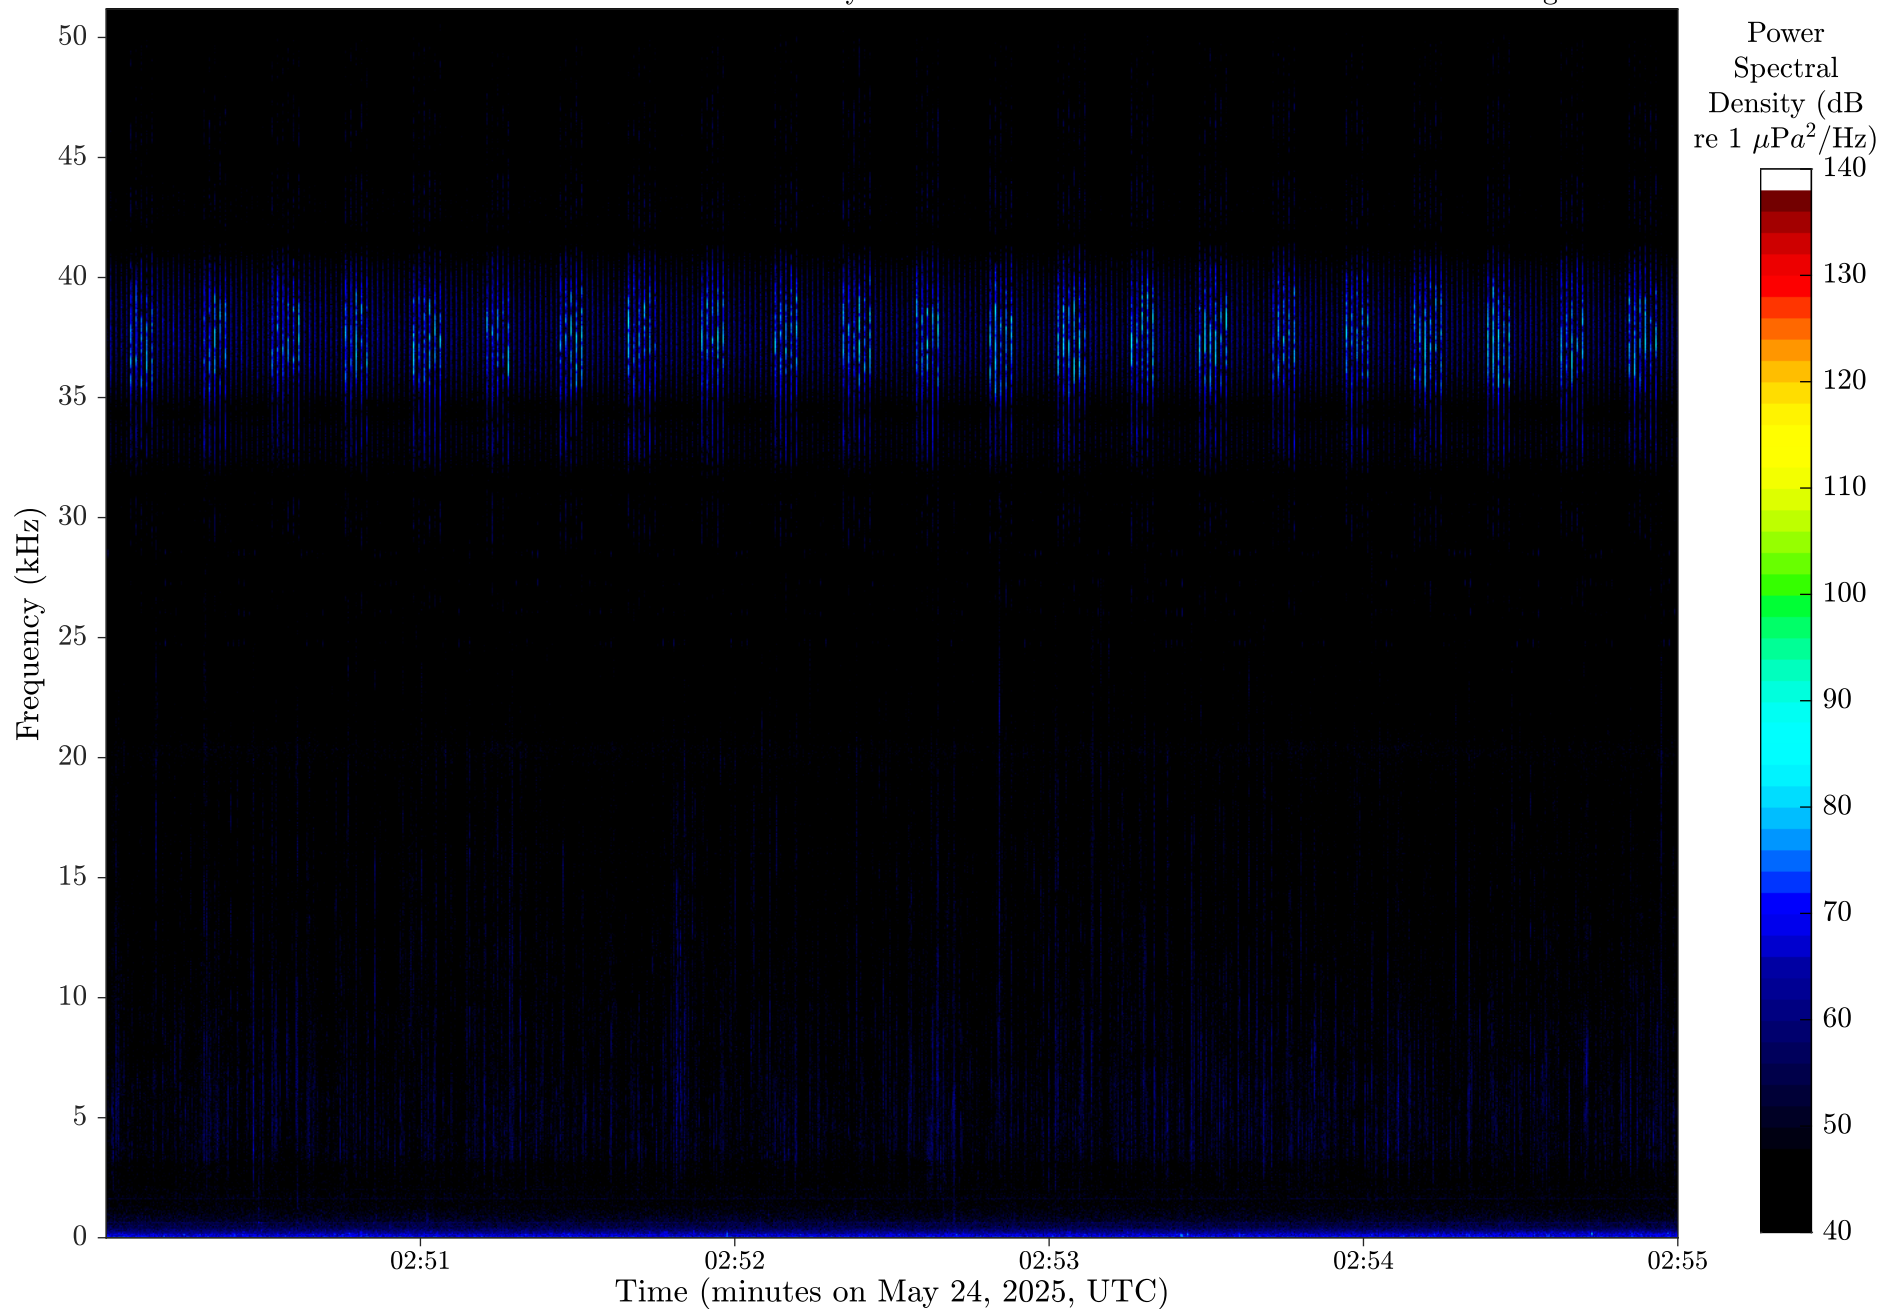


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:23:43 UTC

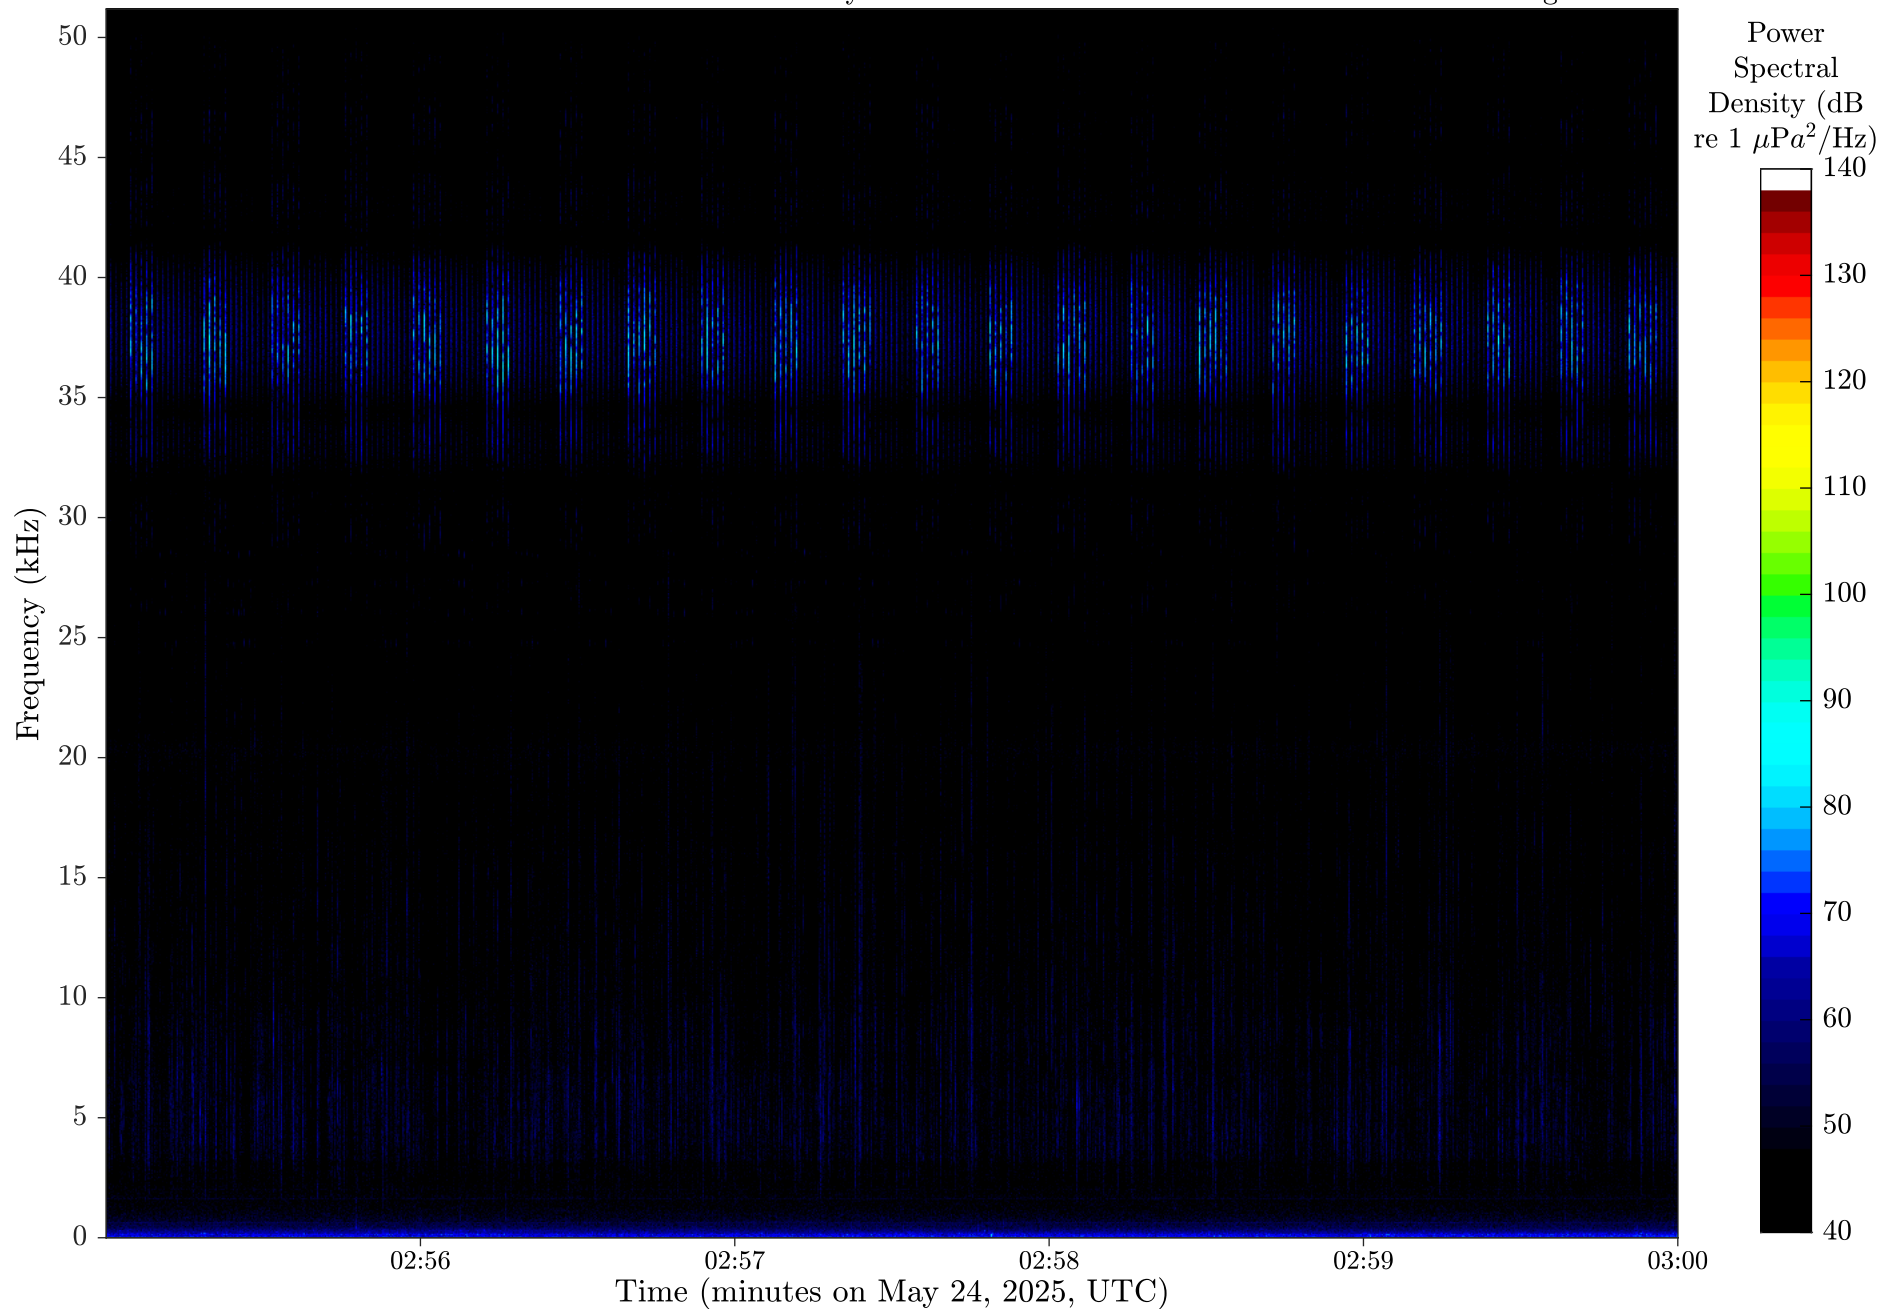

Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:23:52 UTC

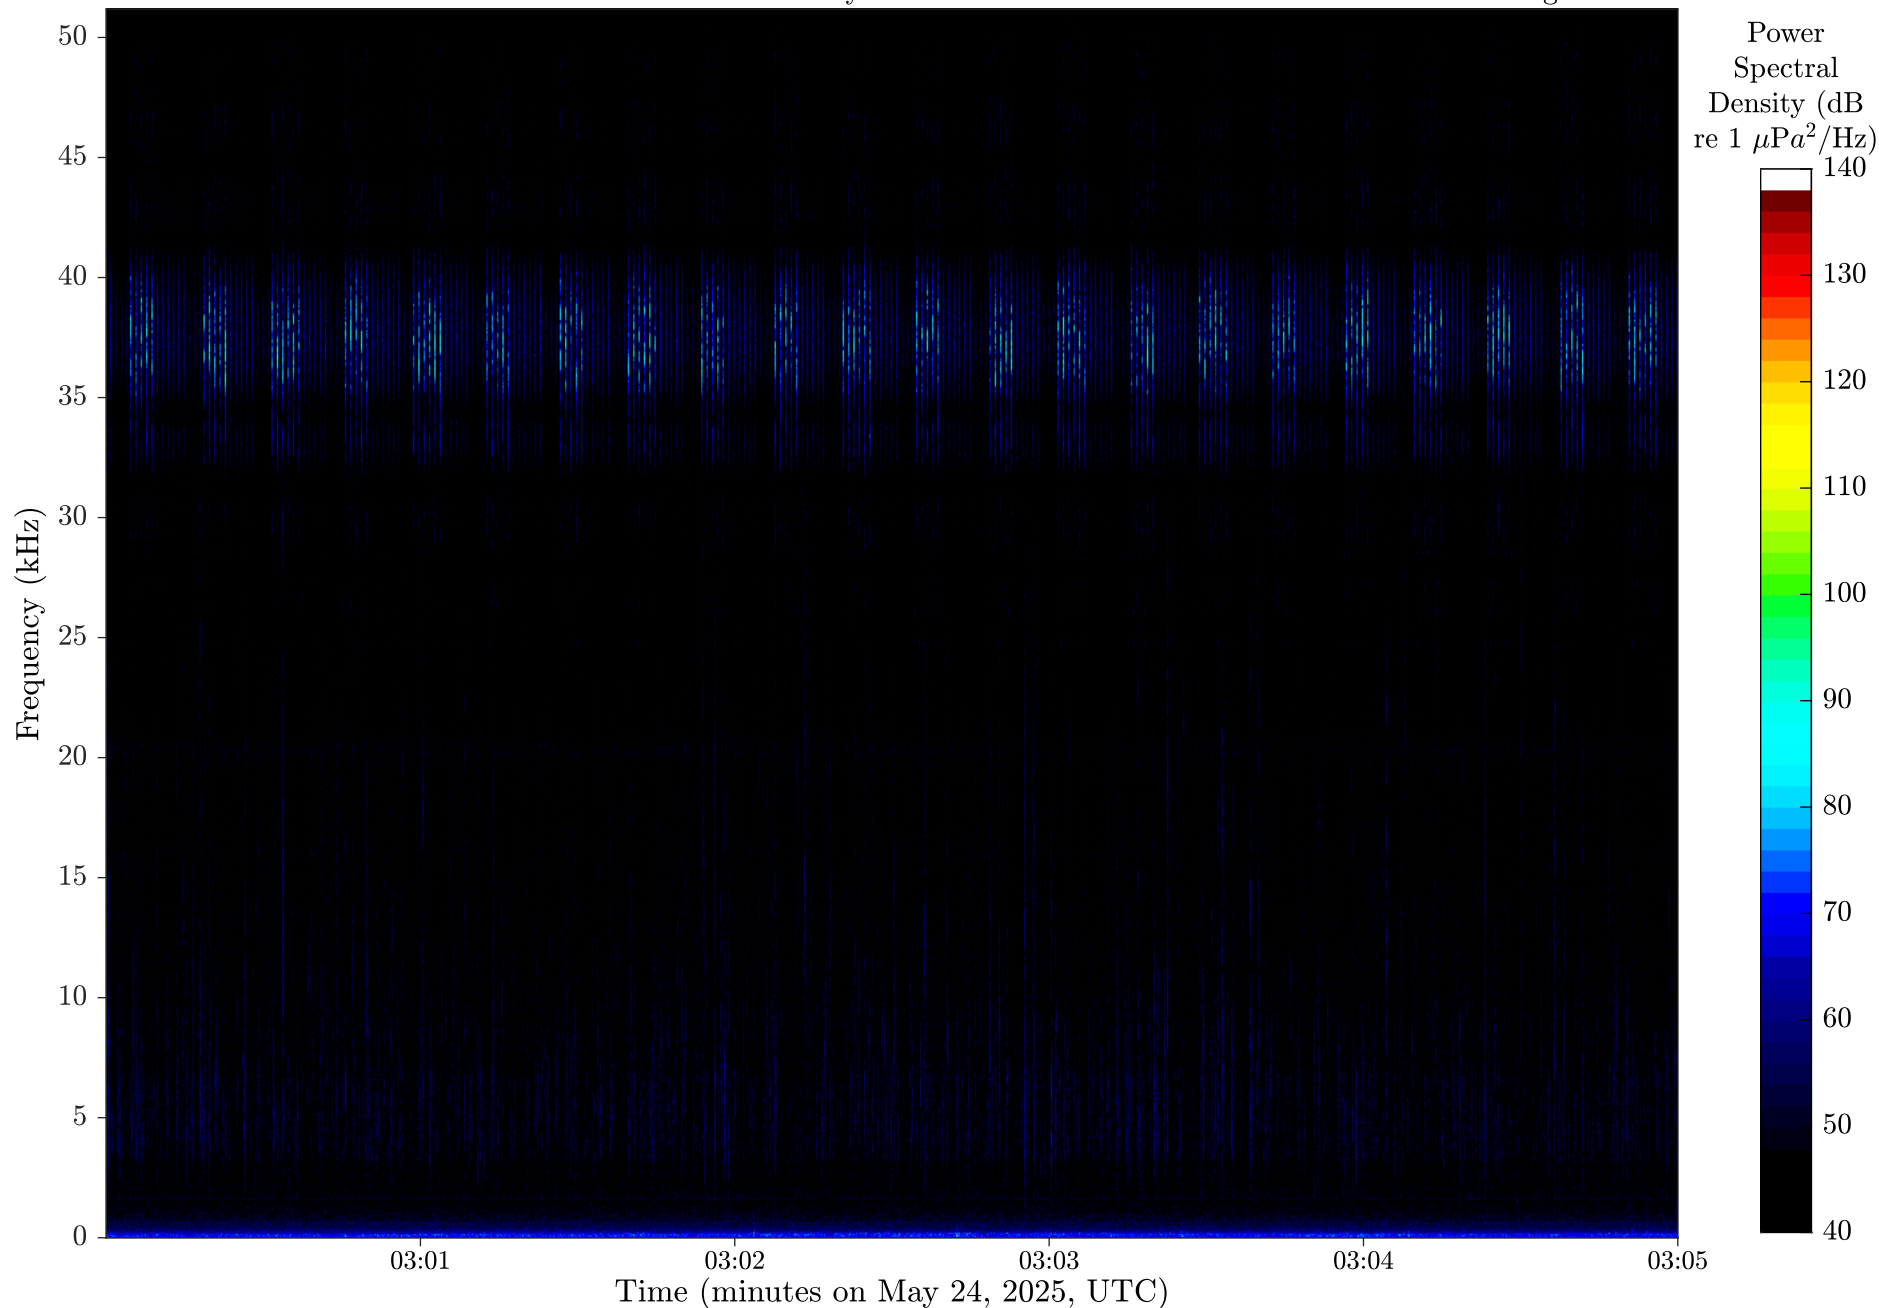

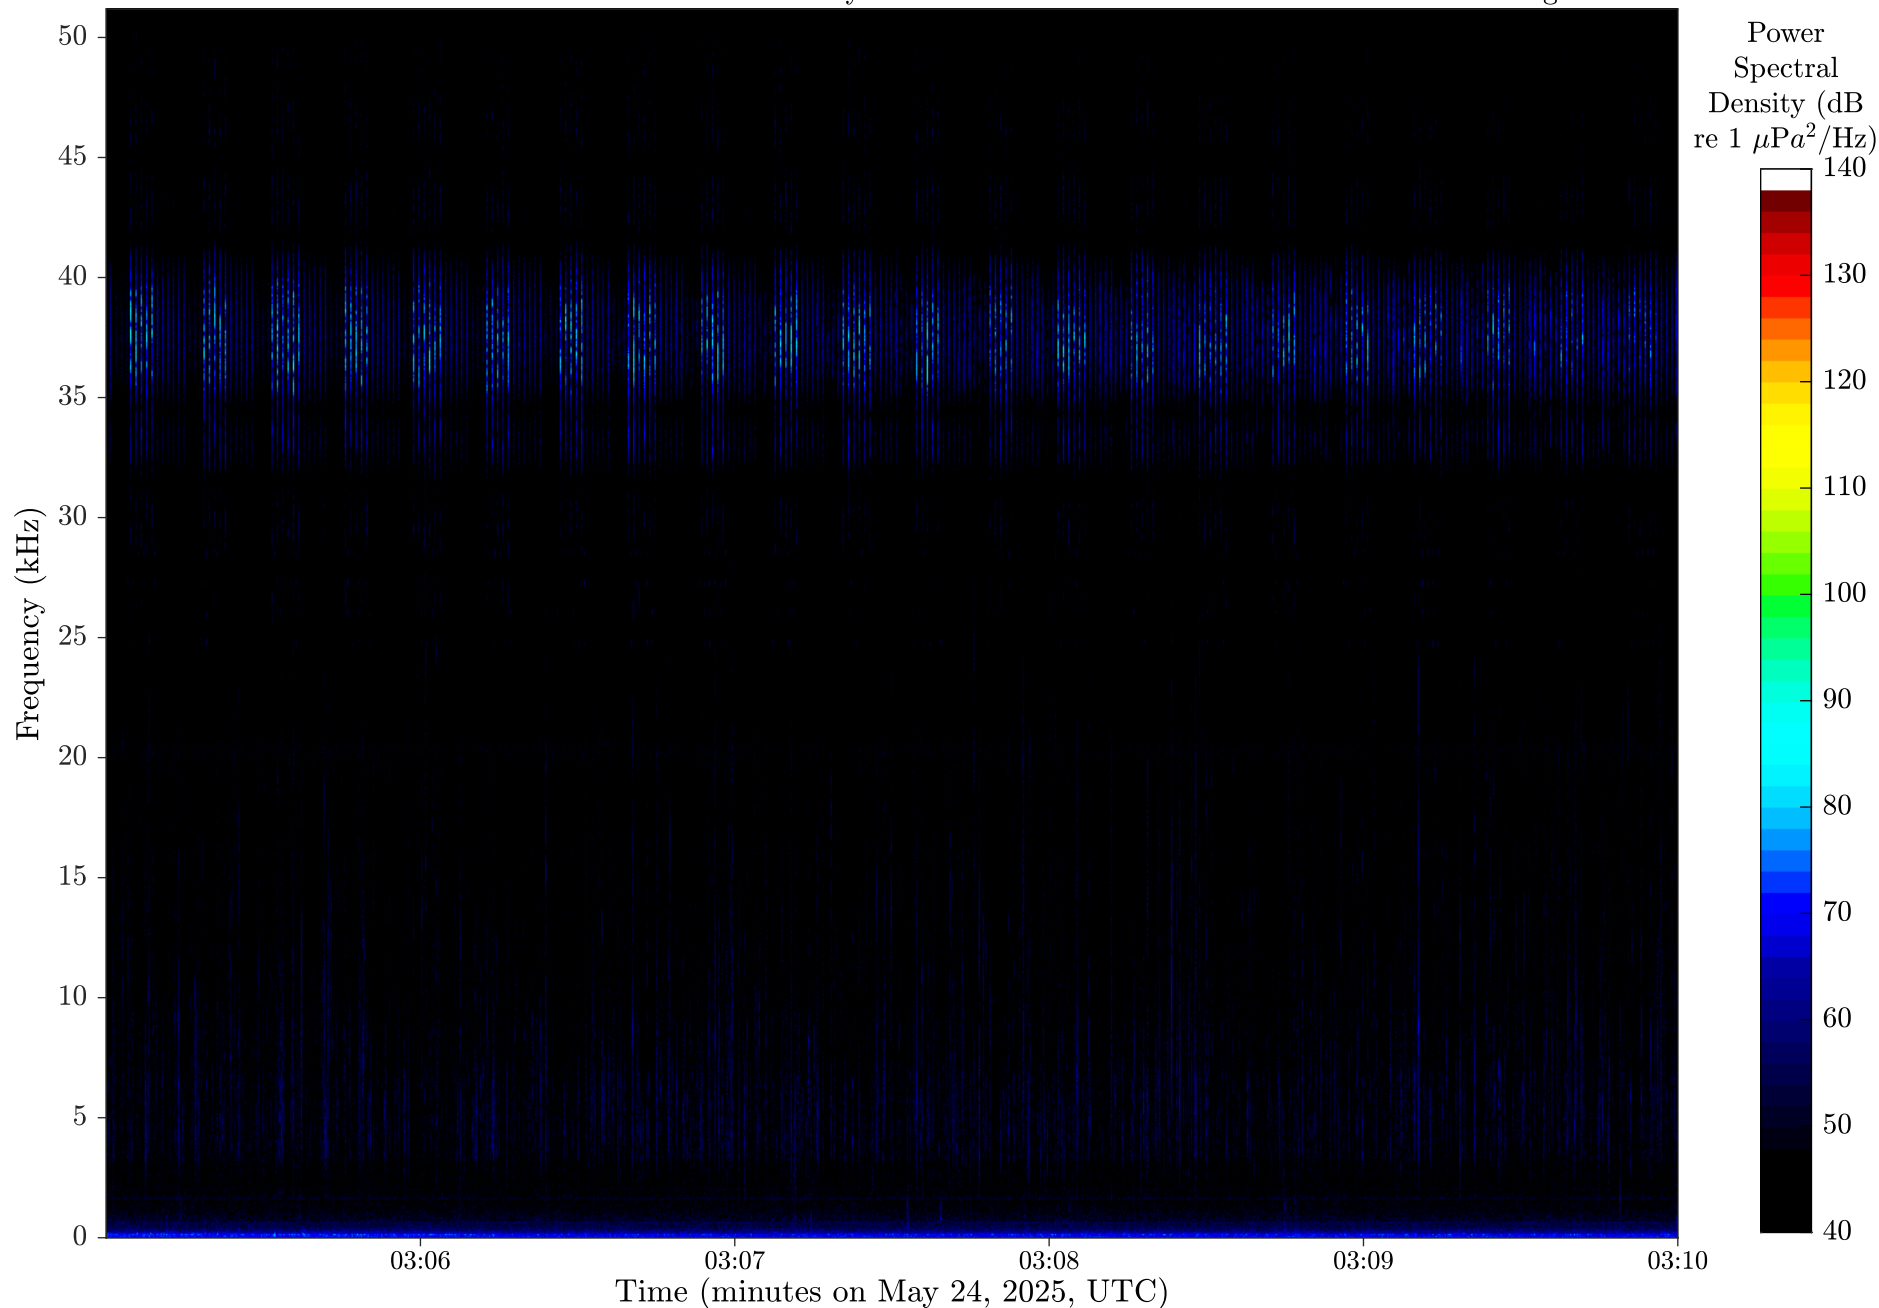


Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:24:08 UTC

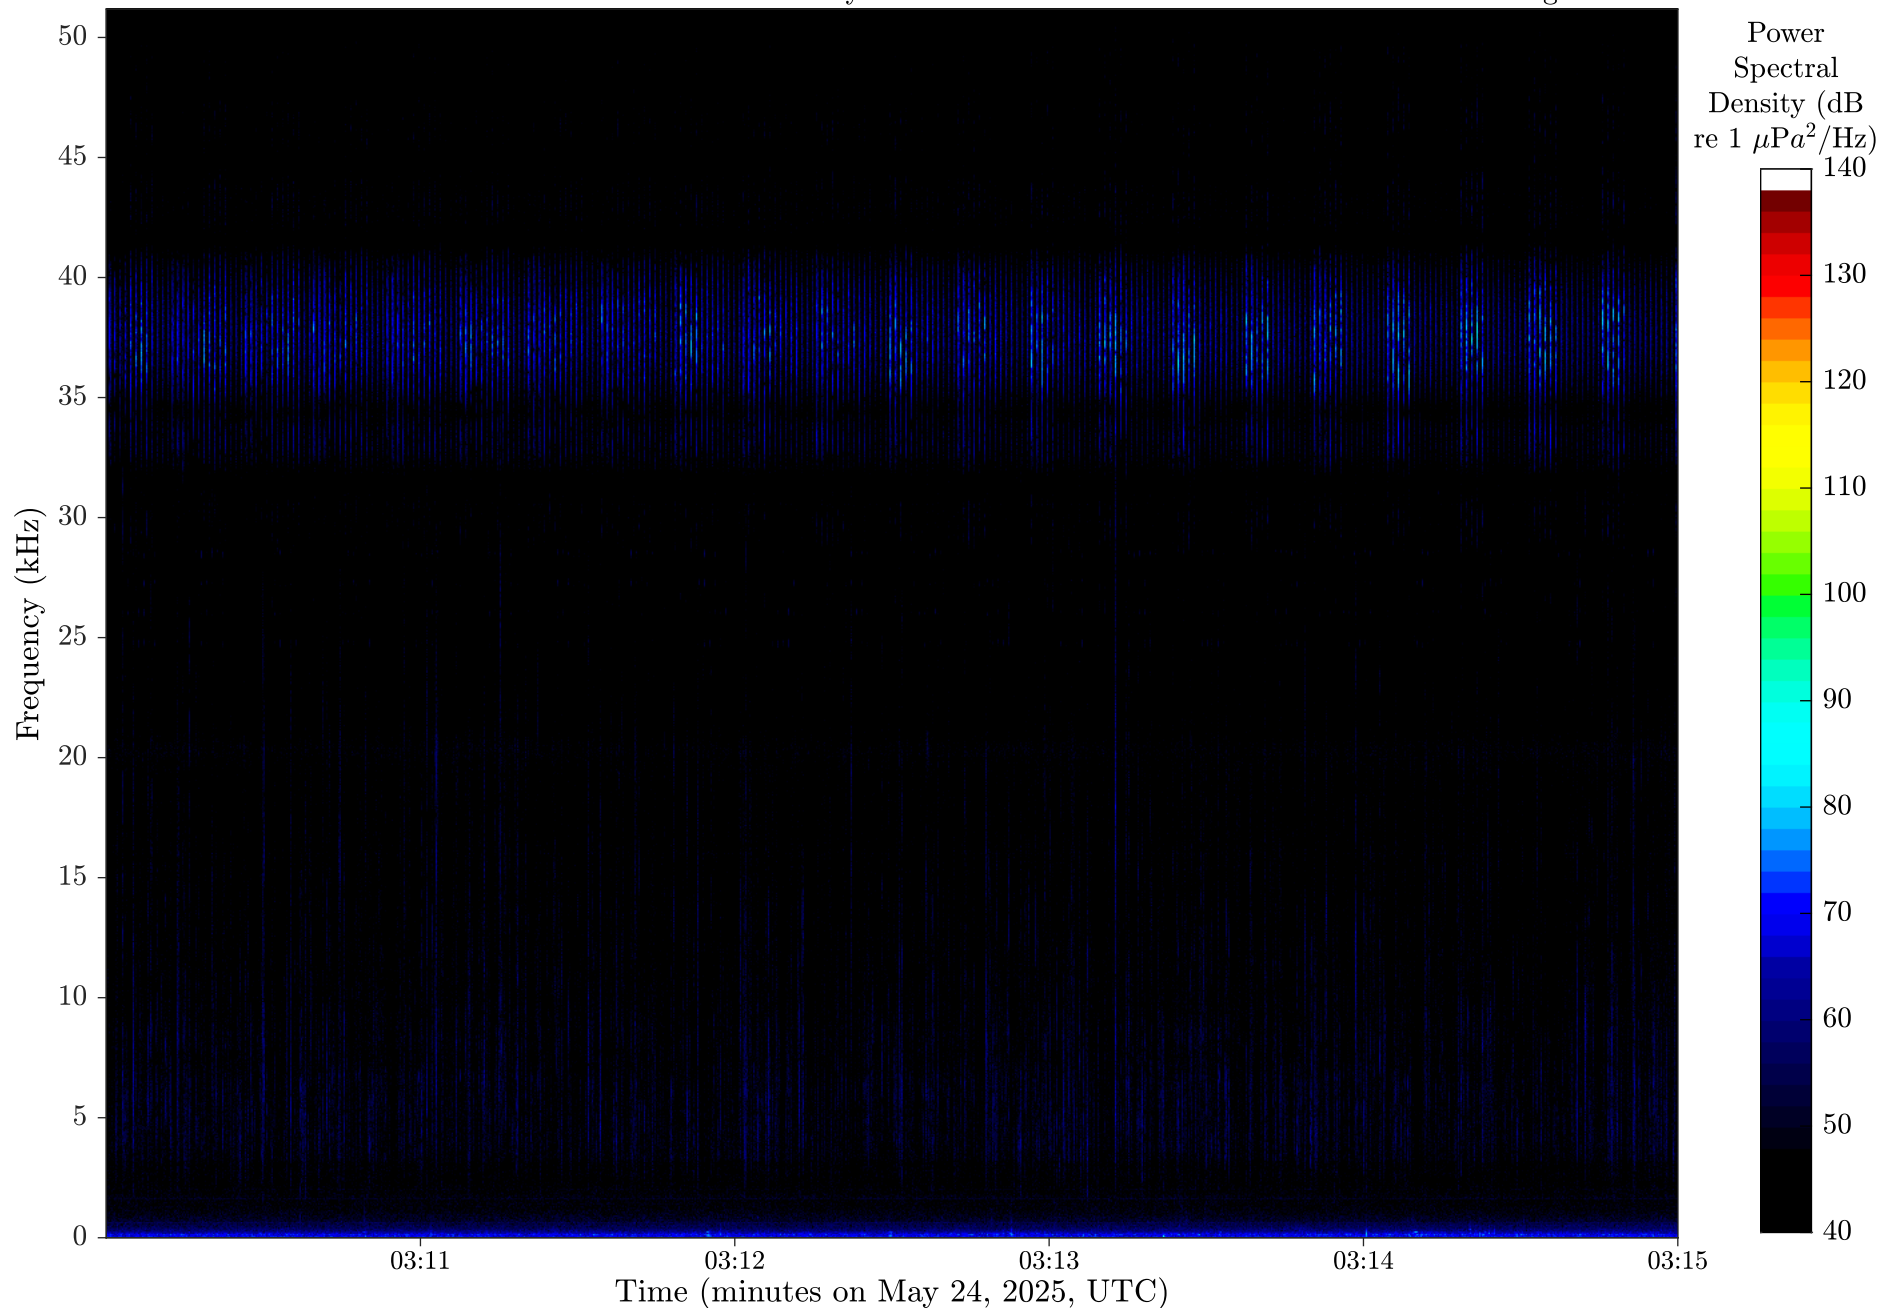

Comments: 33.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:24:17 UTC

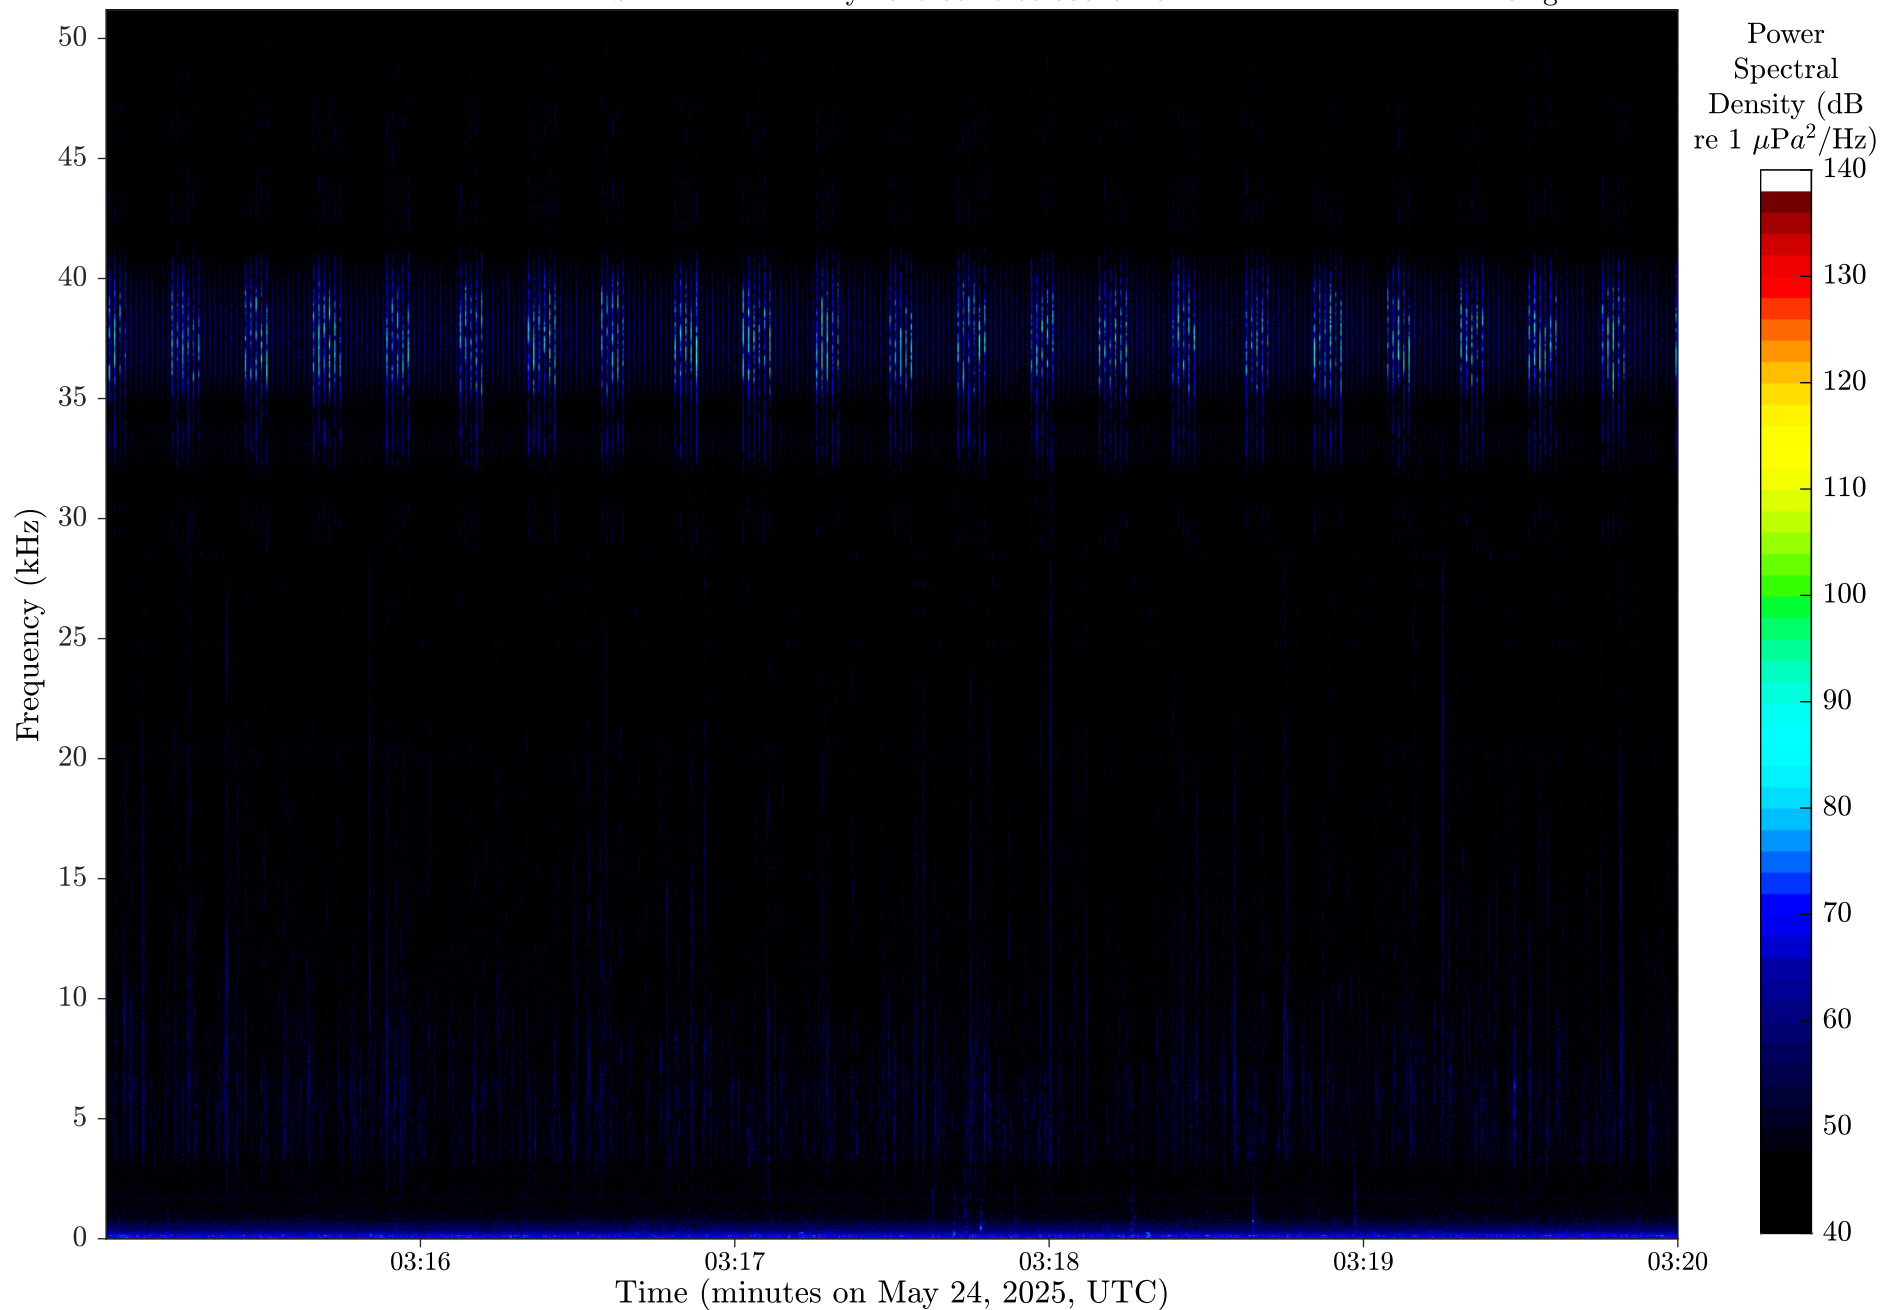


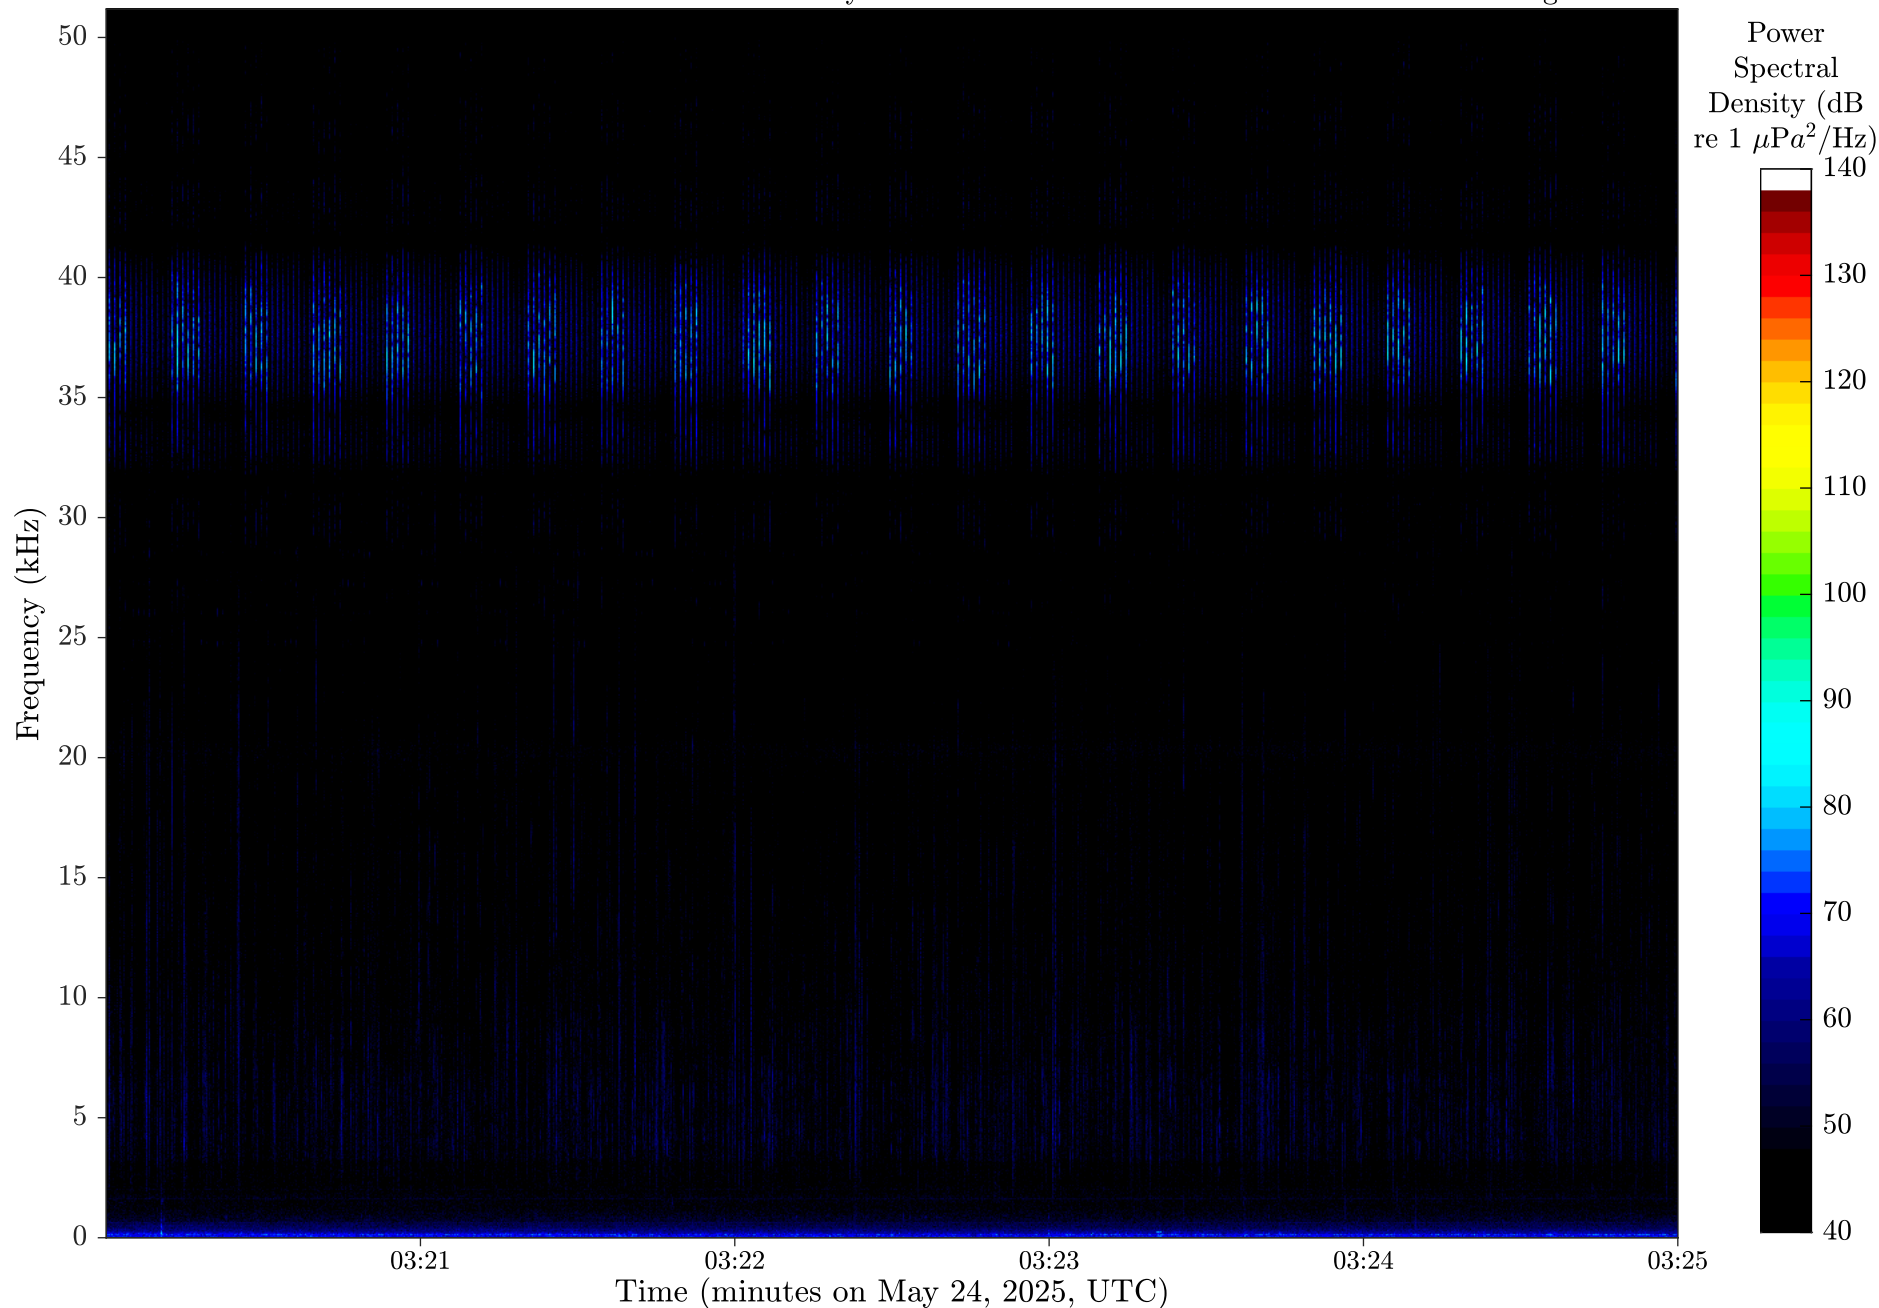

Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:24:33 UTC

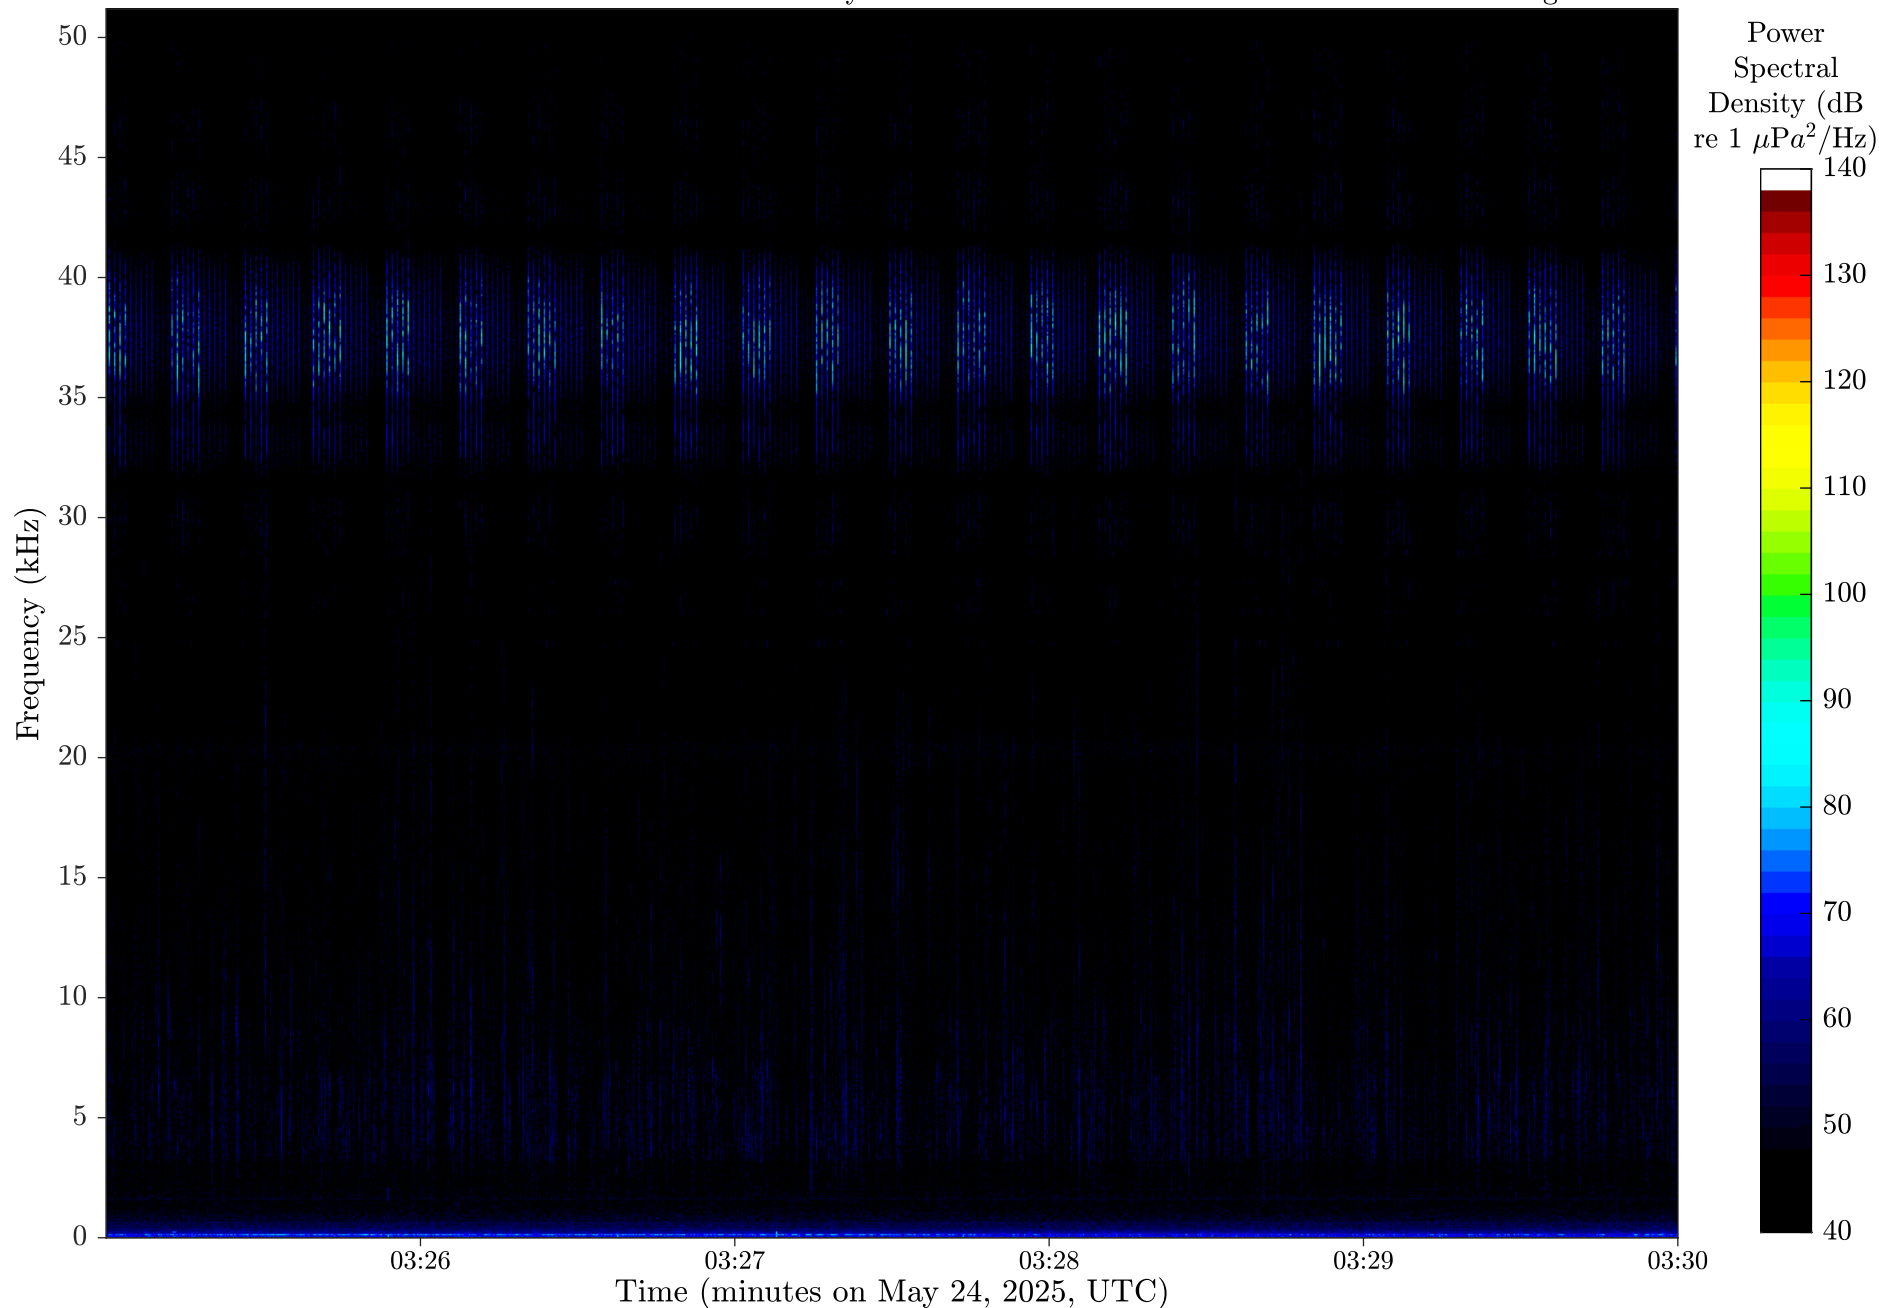

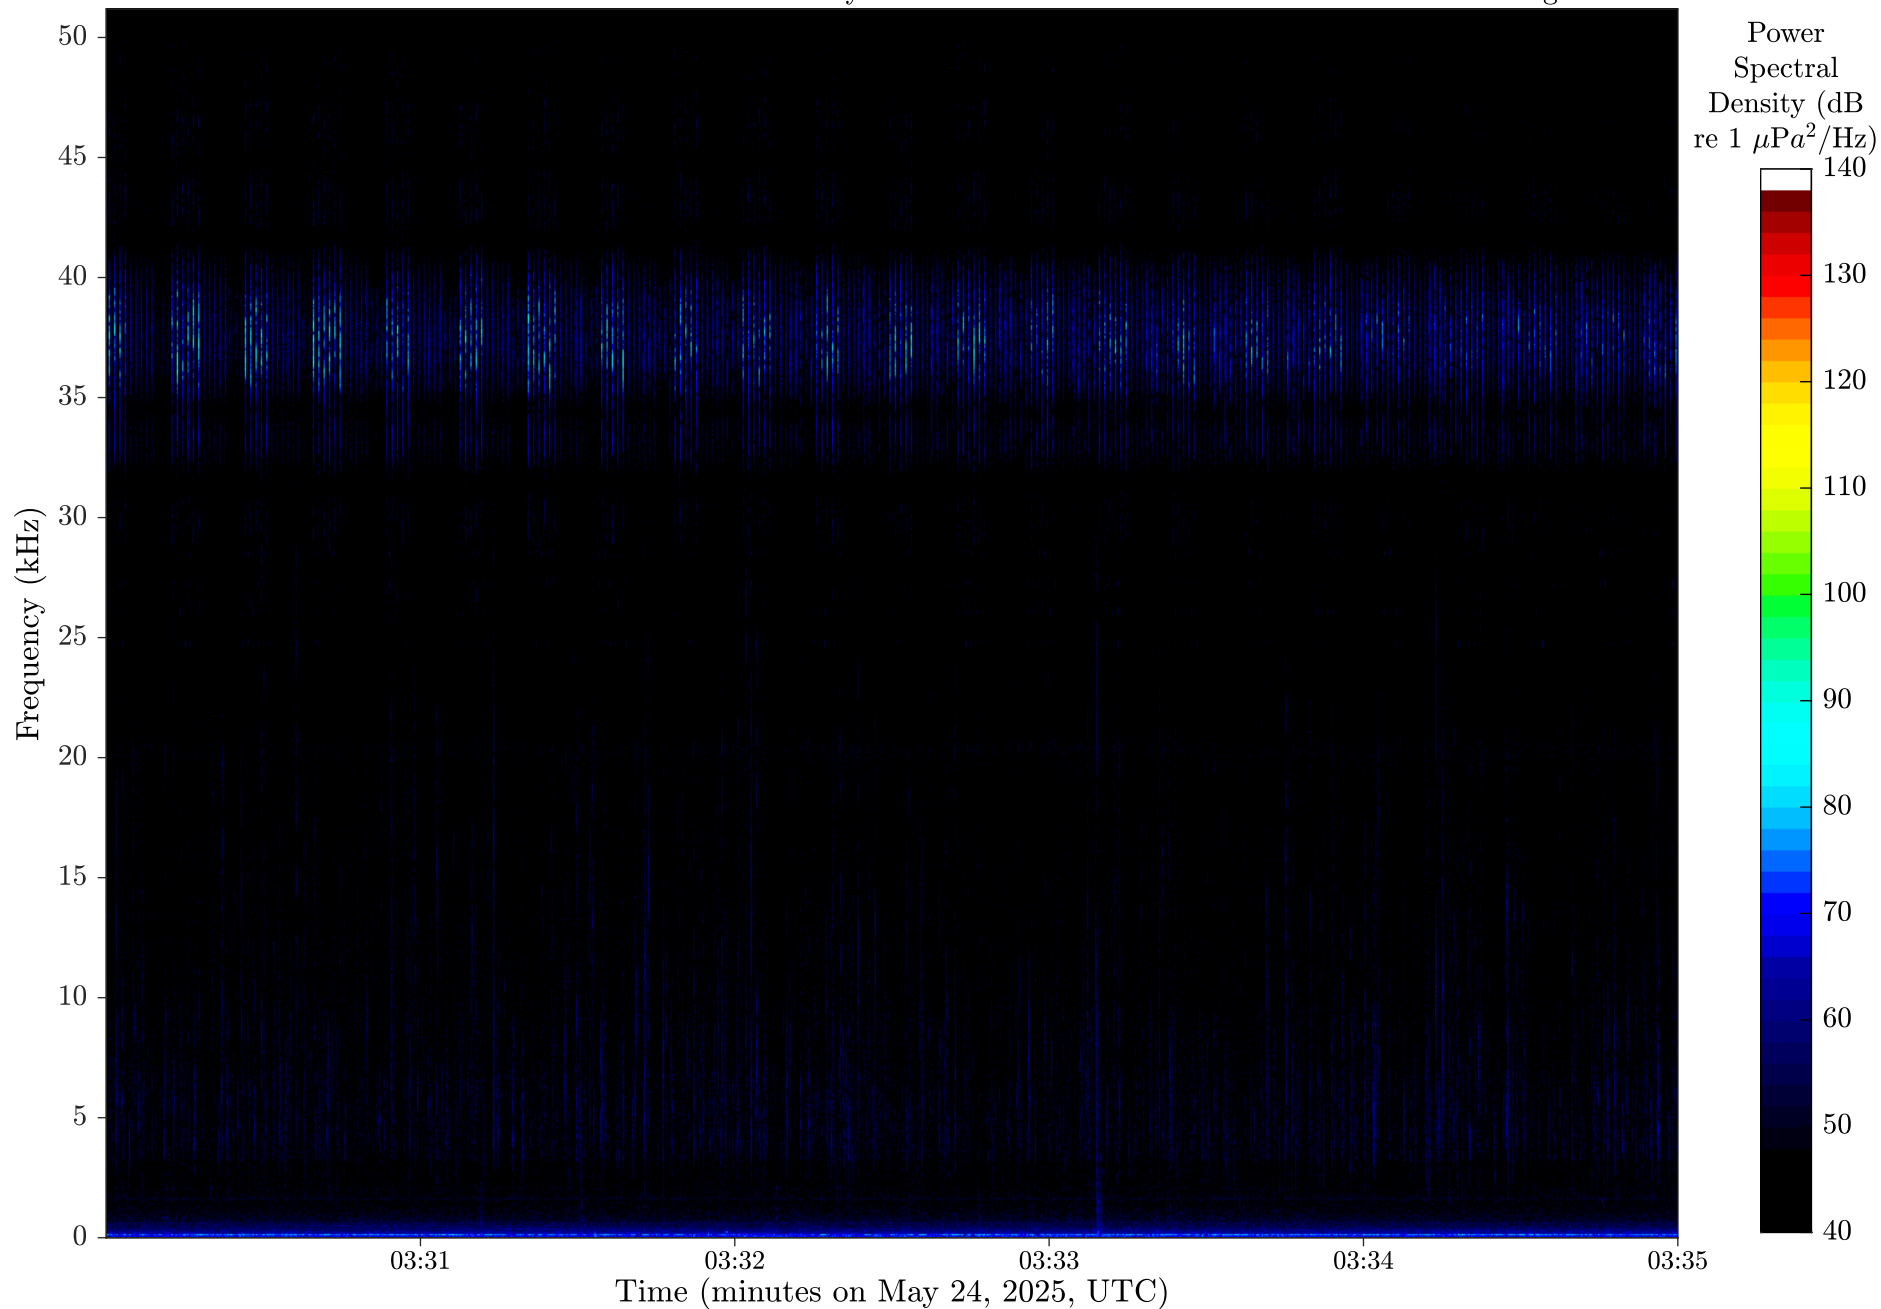


Comments: 34.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:24:50 UTC

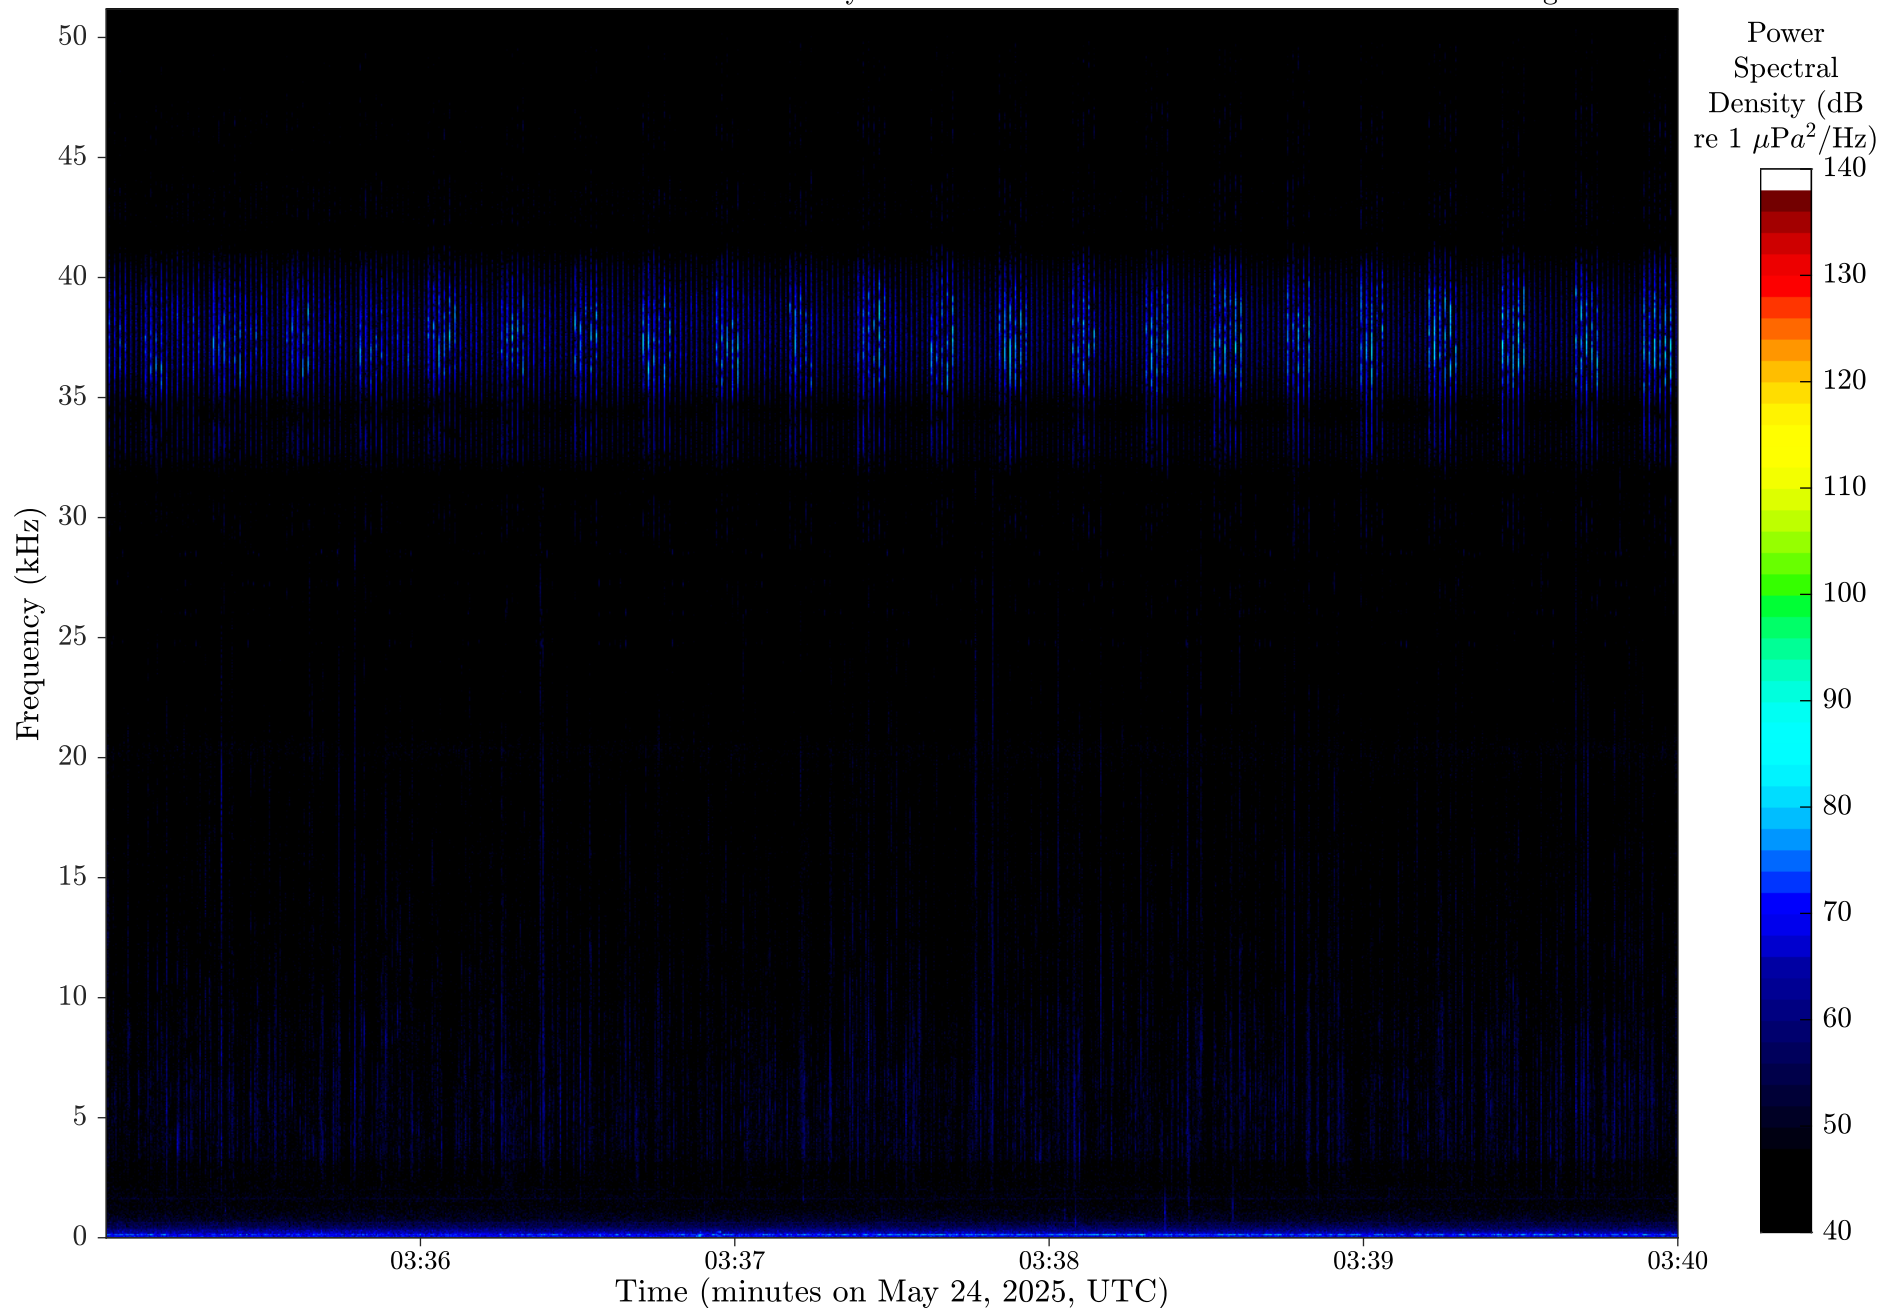

Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:24:58 UTC

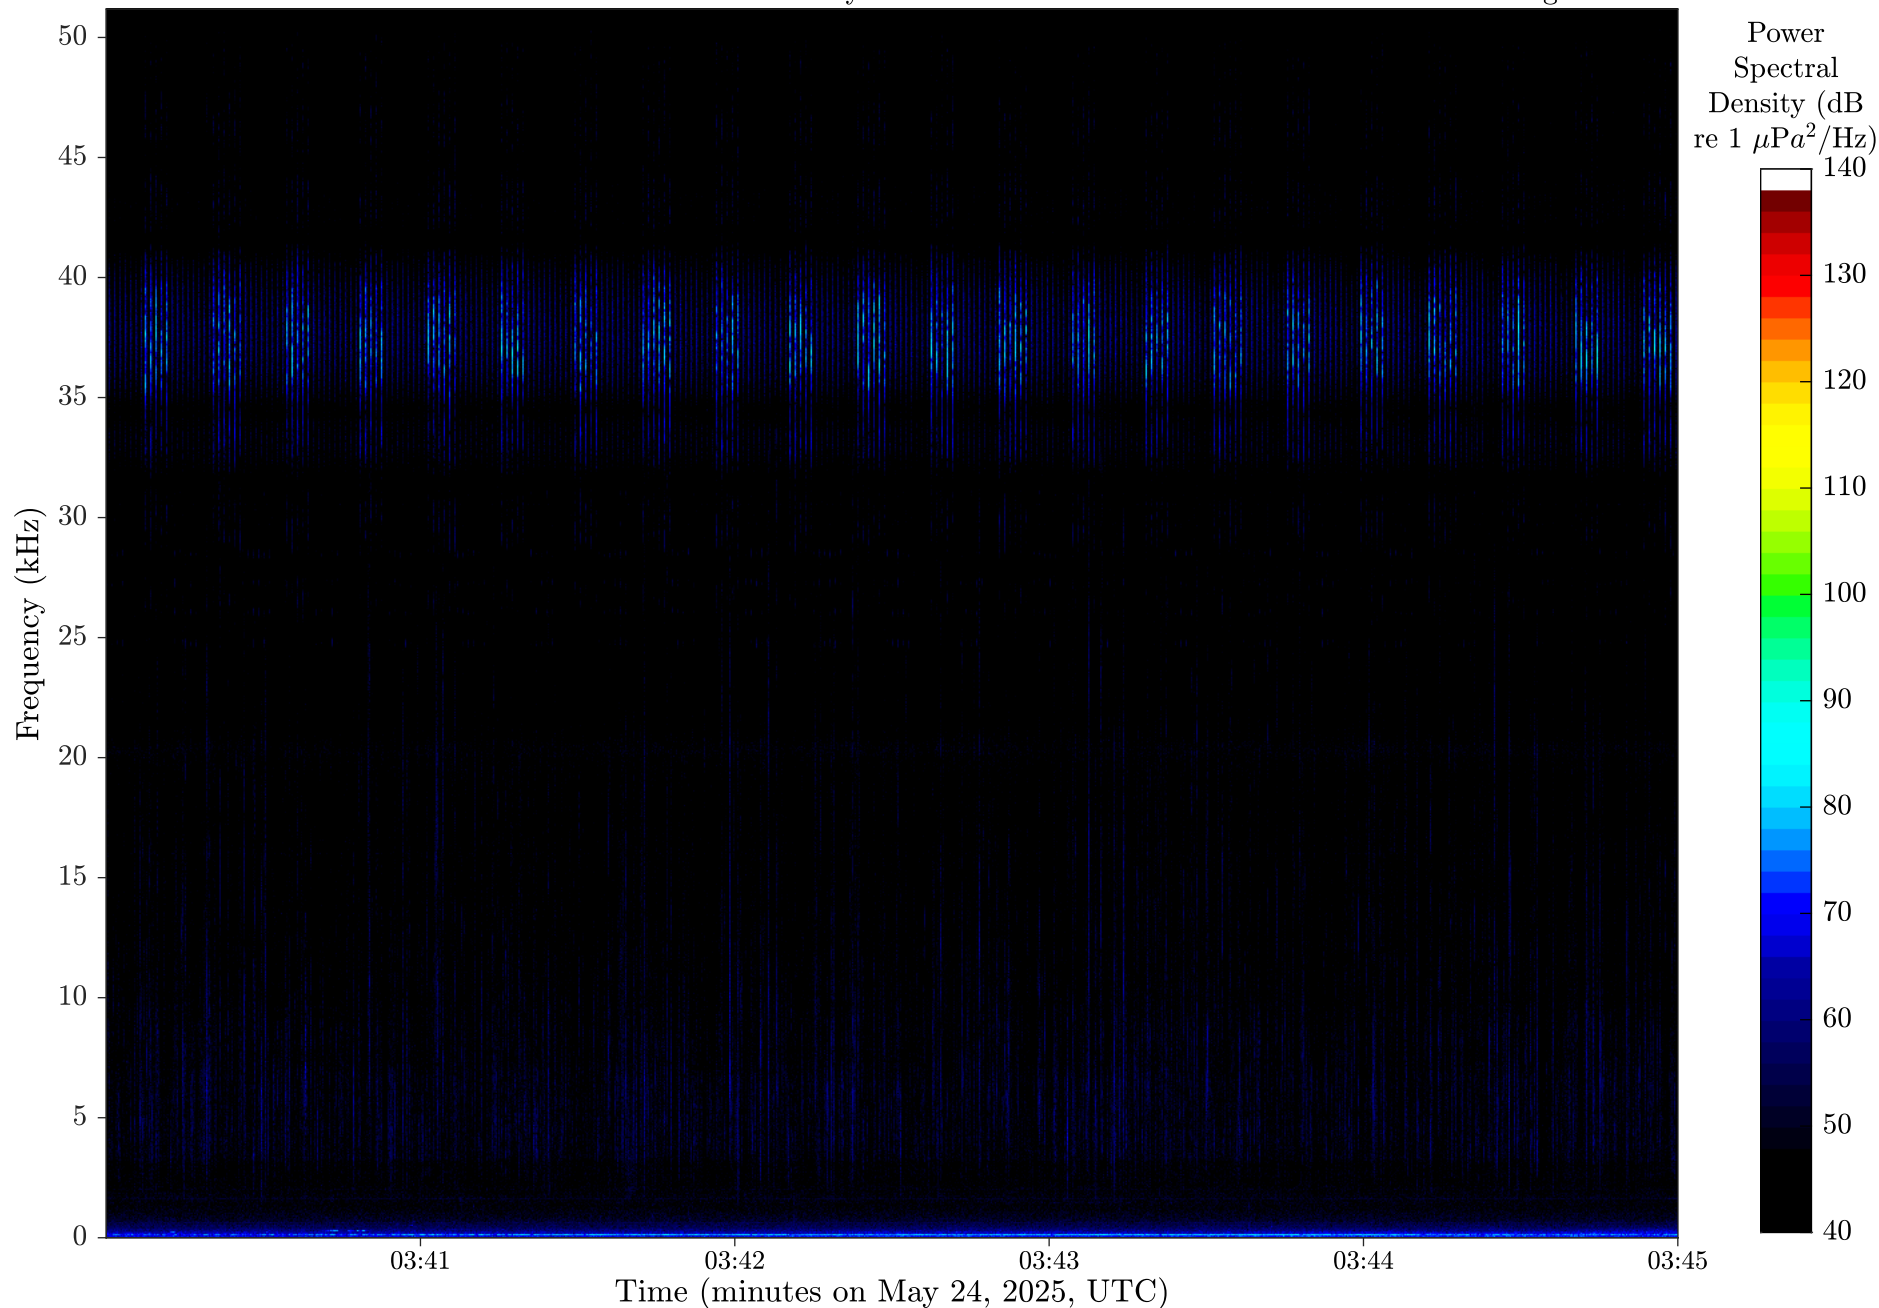

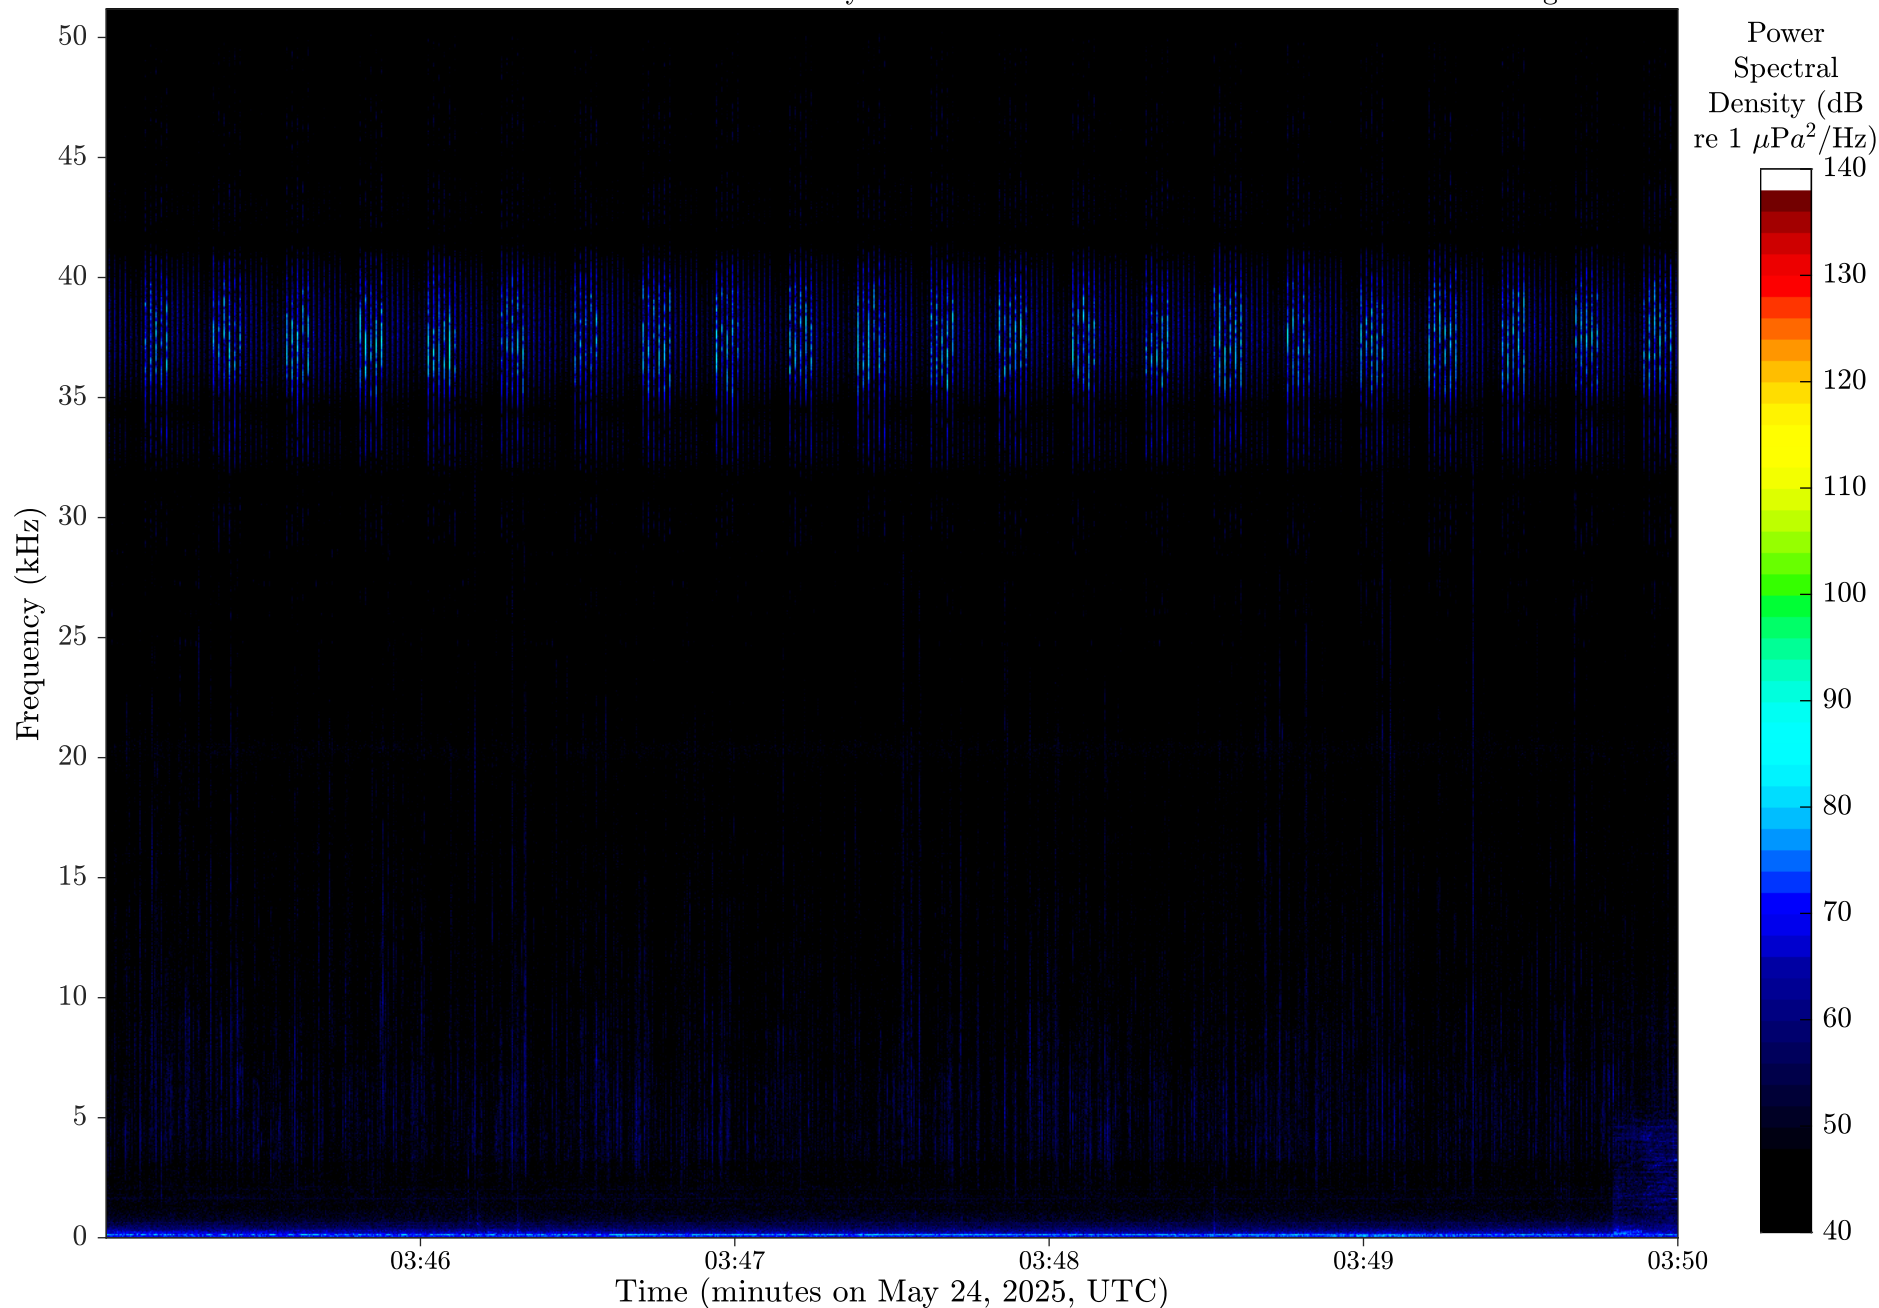


Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:15 UTC

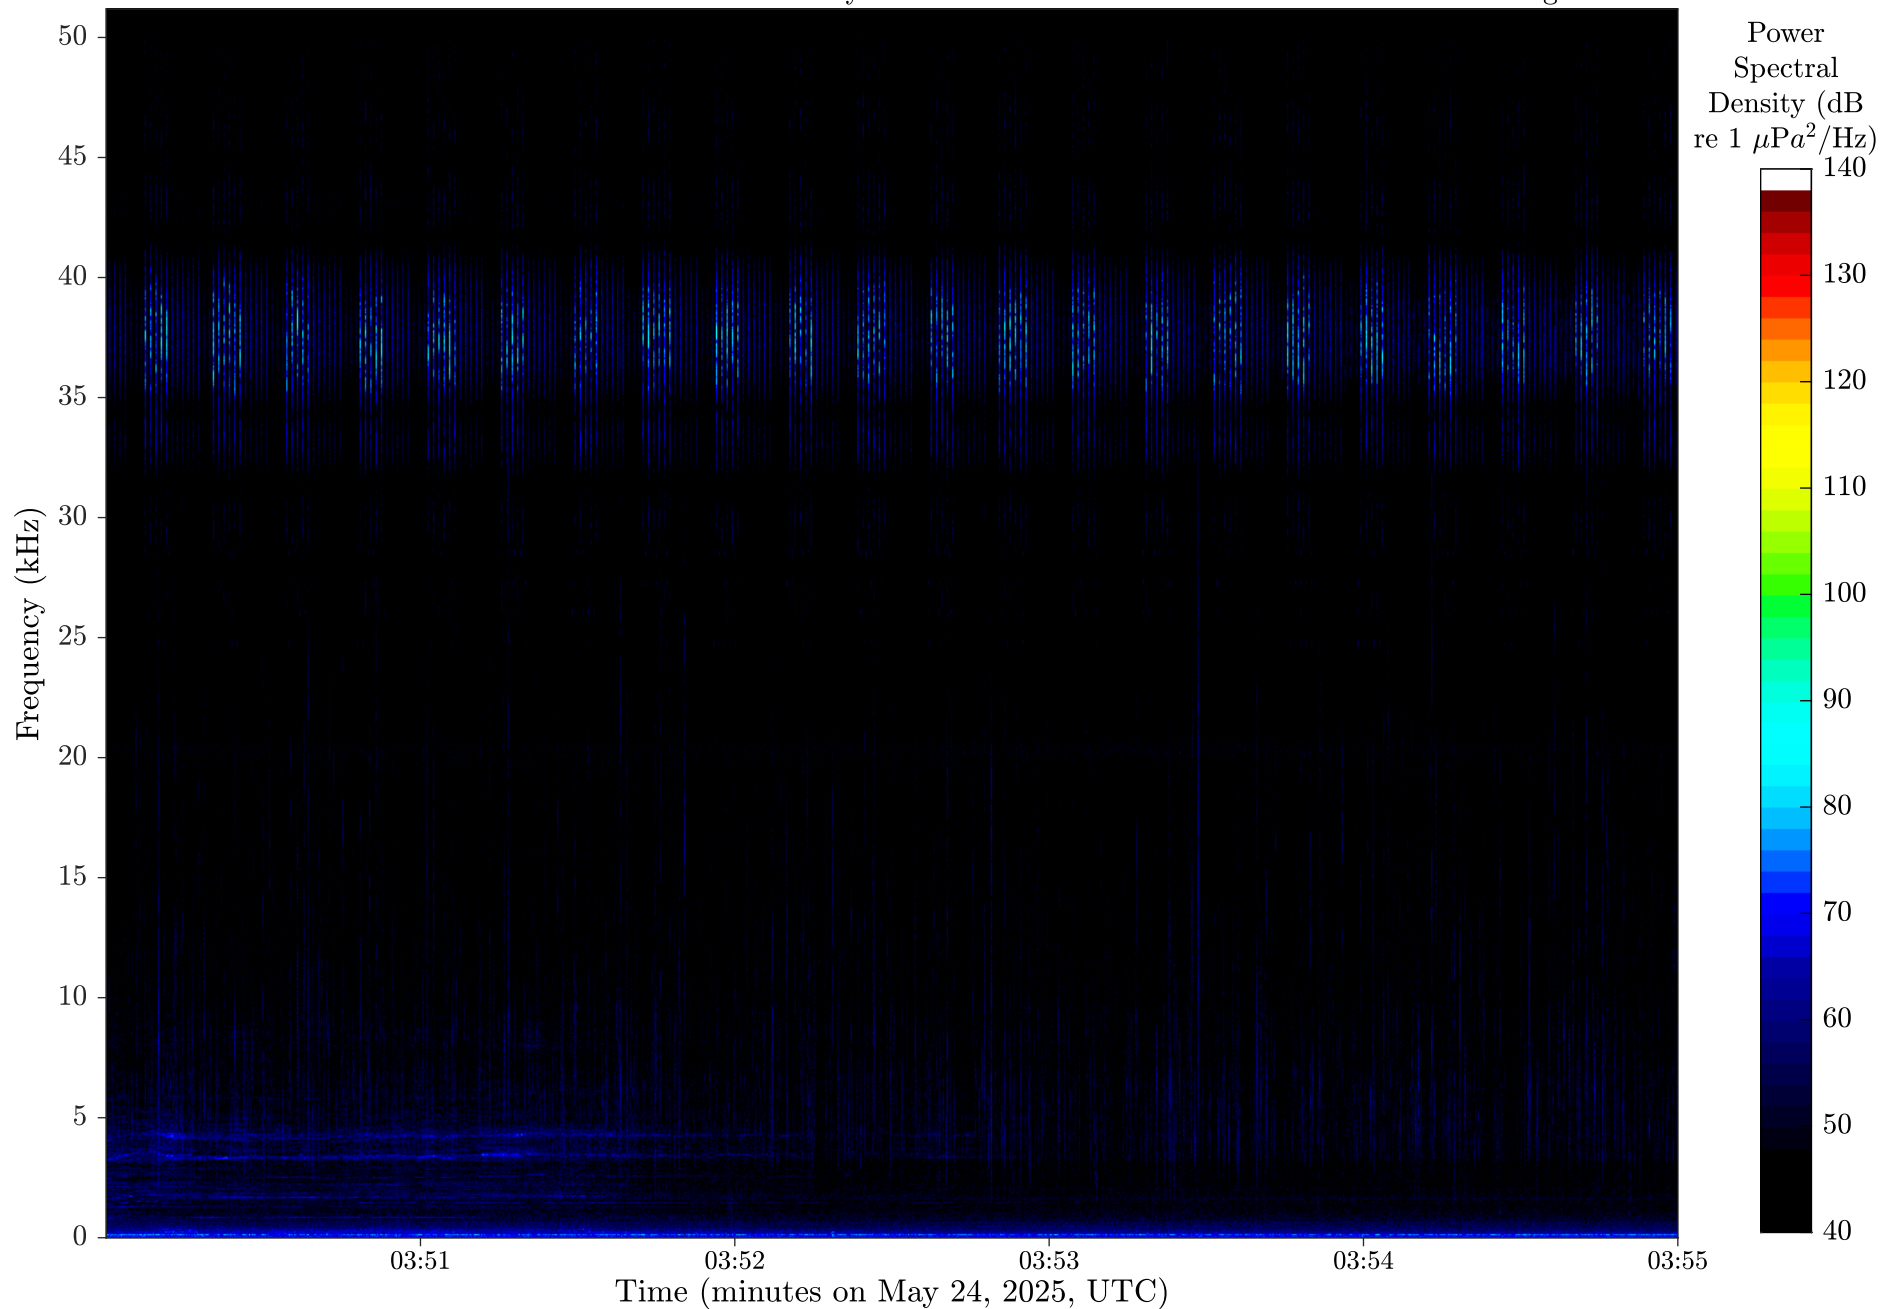


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:24 UTC

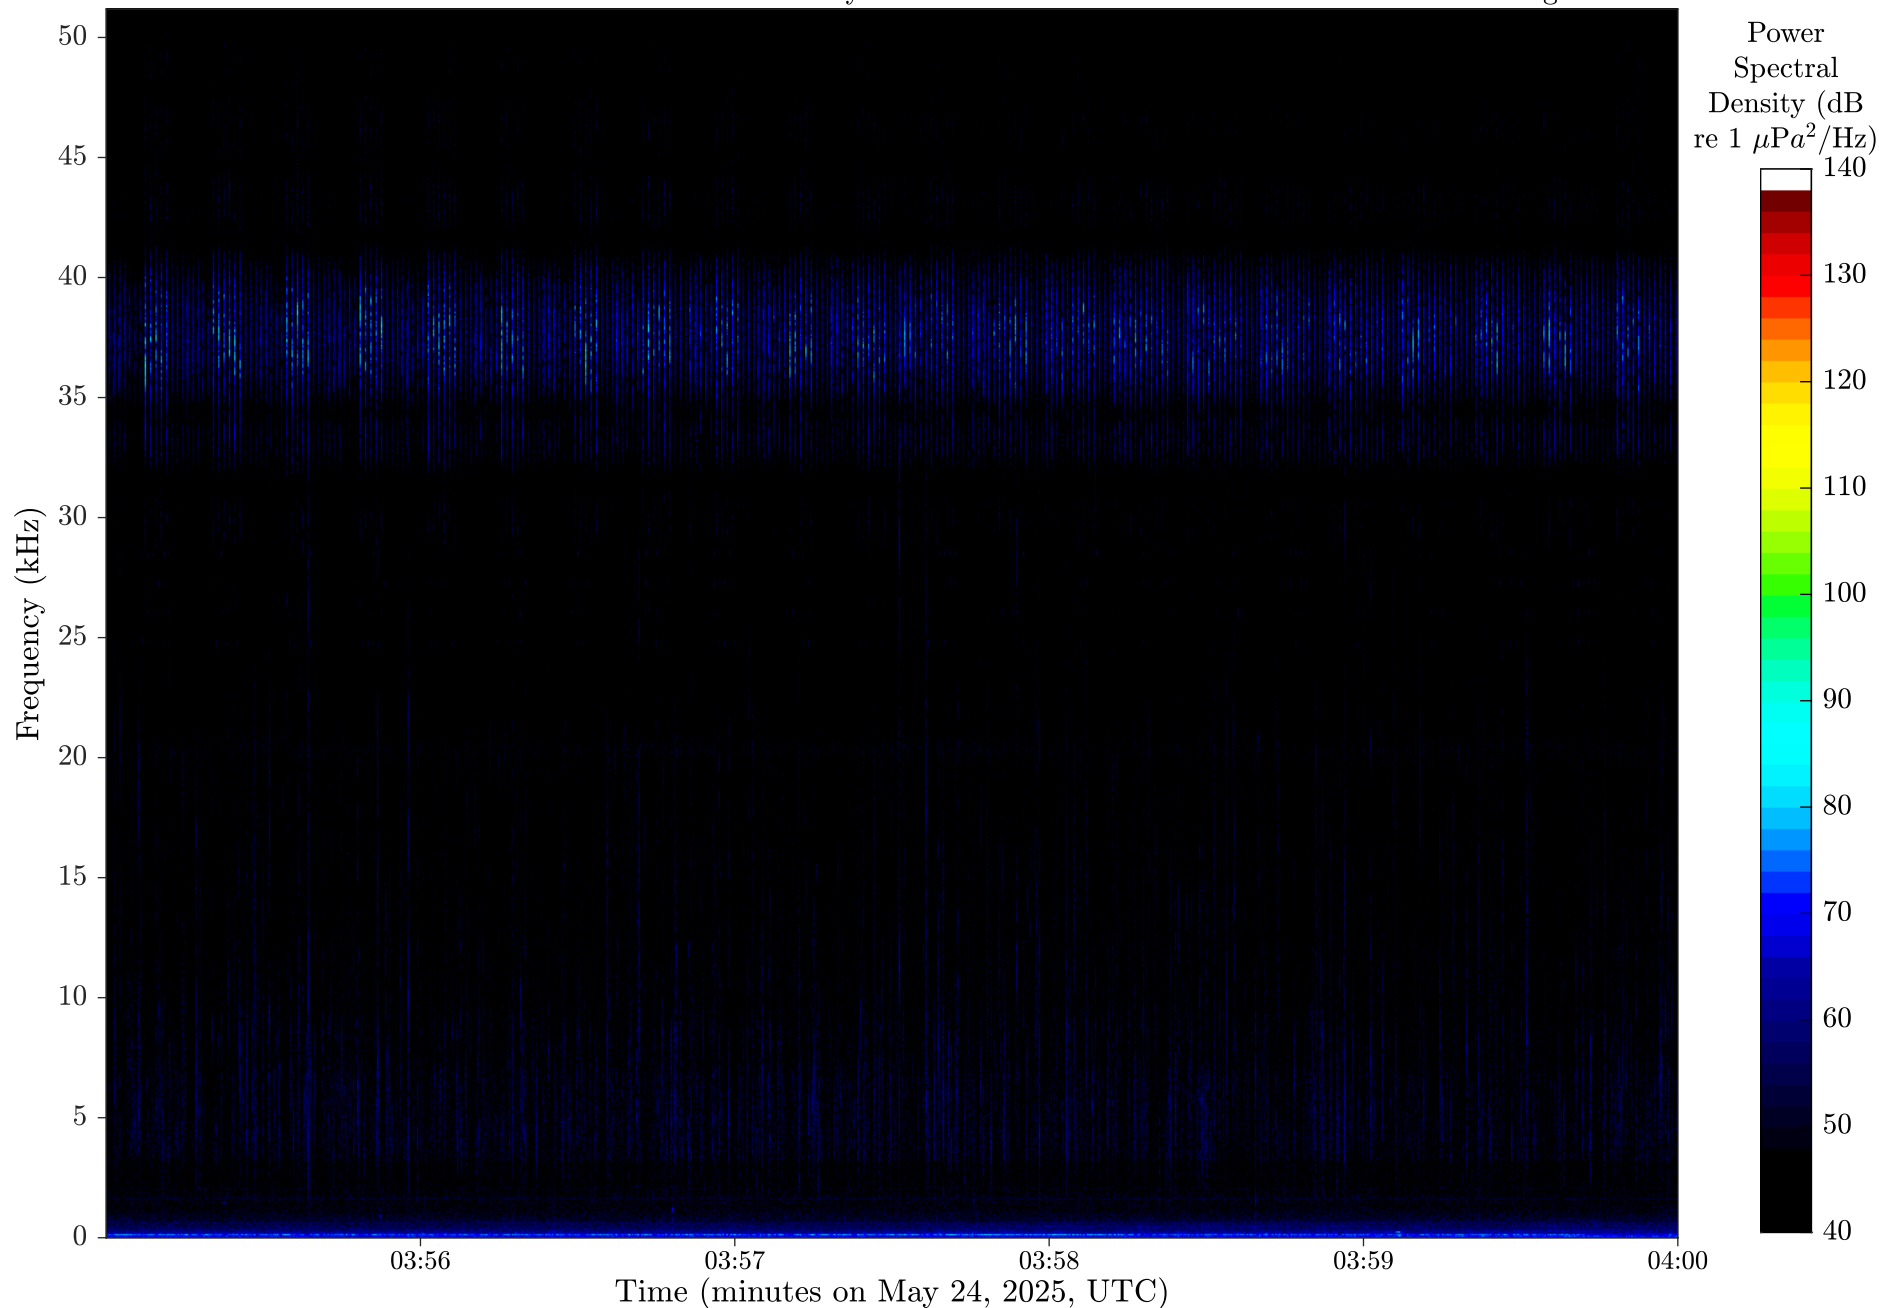


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:32 UTC

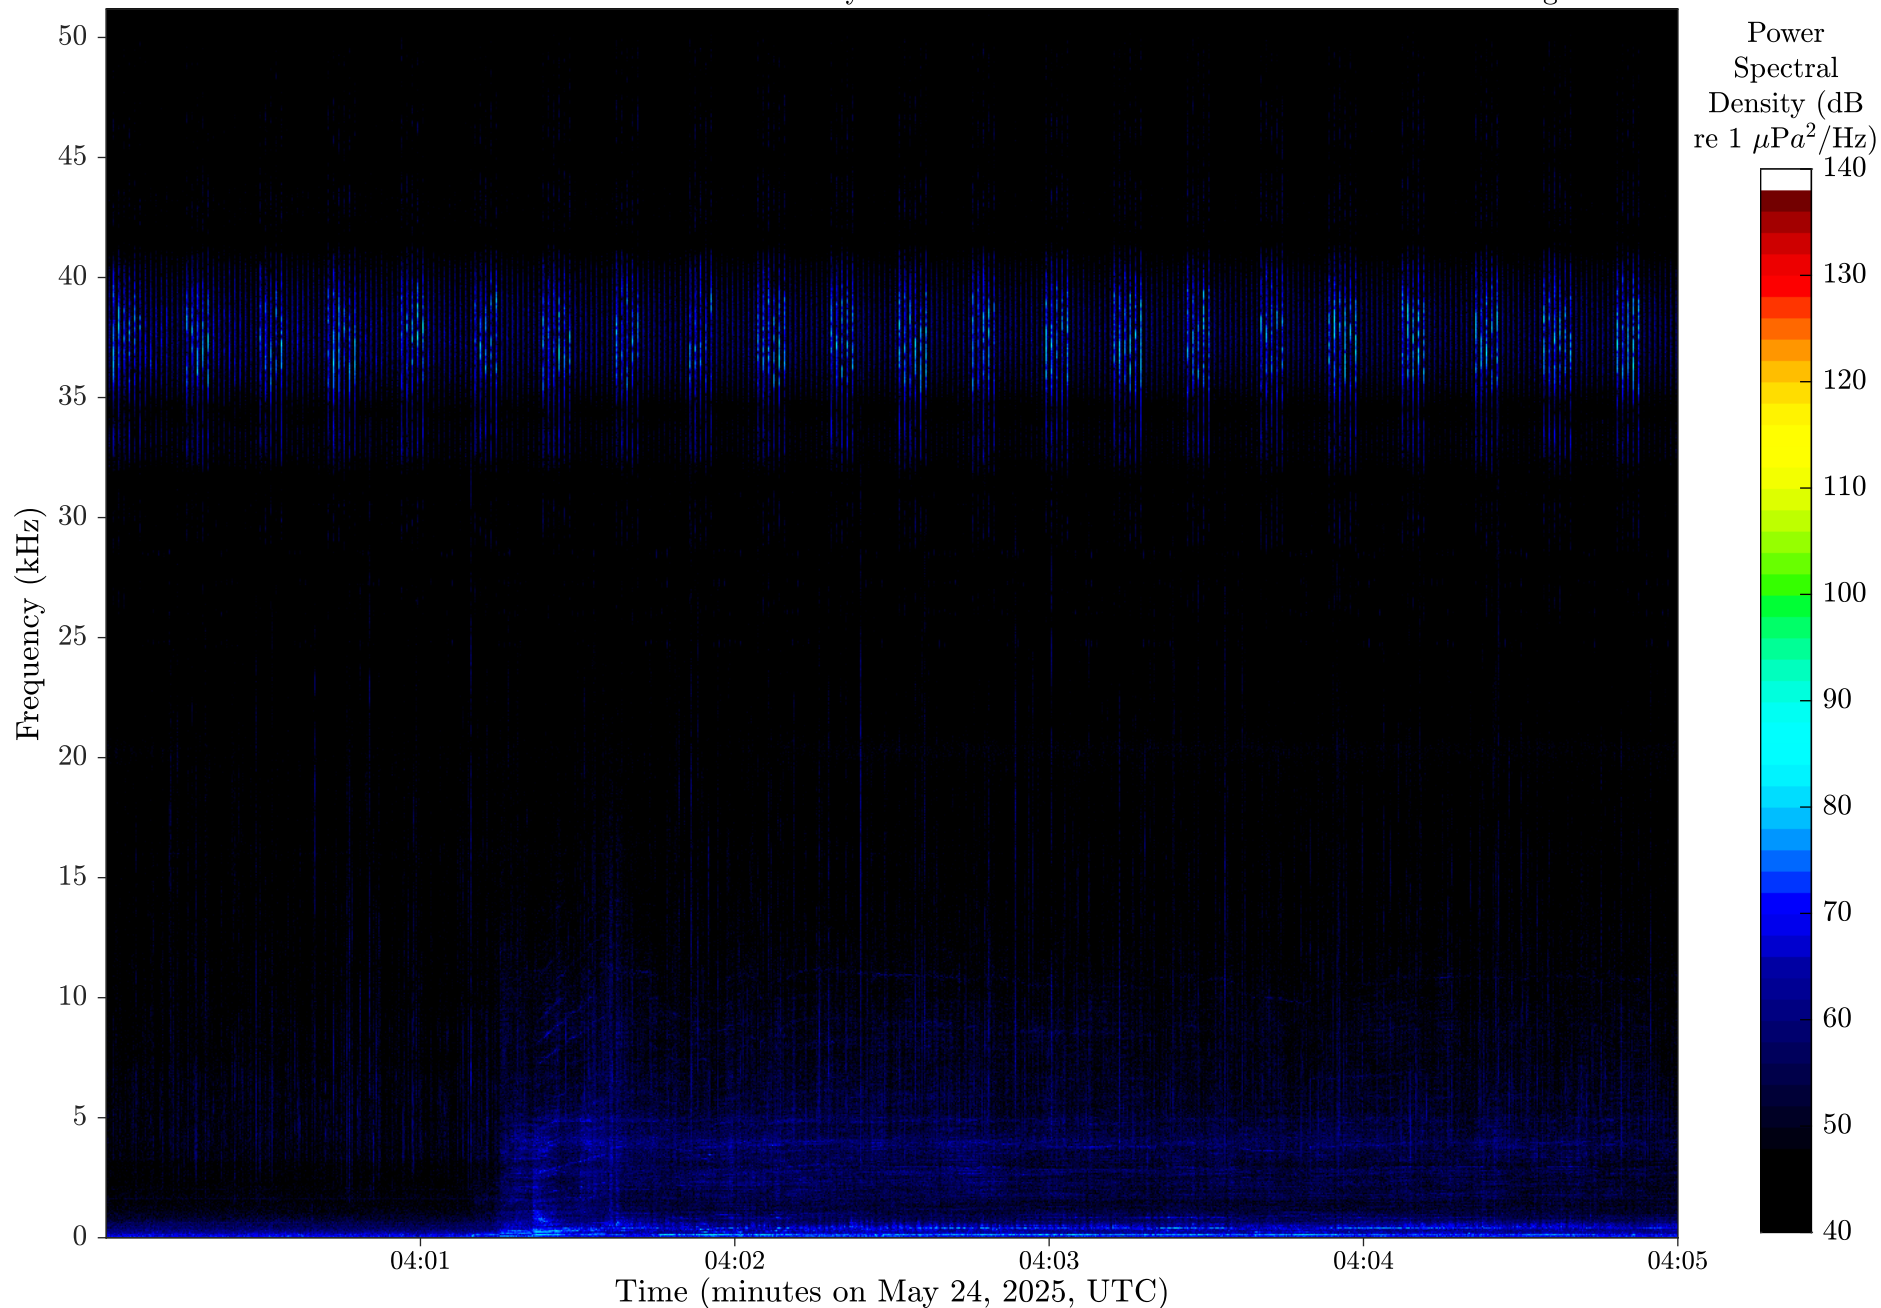


Comments: 32.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:41 UTC

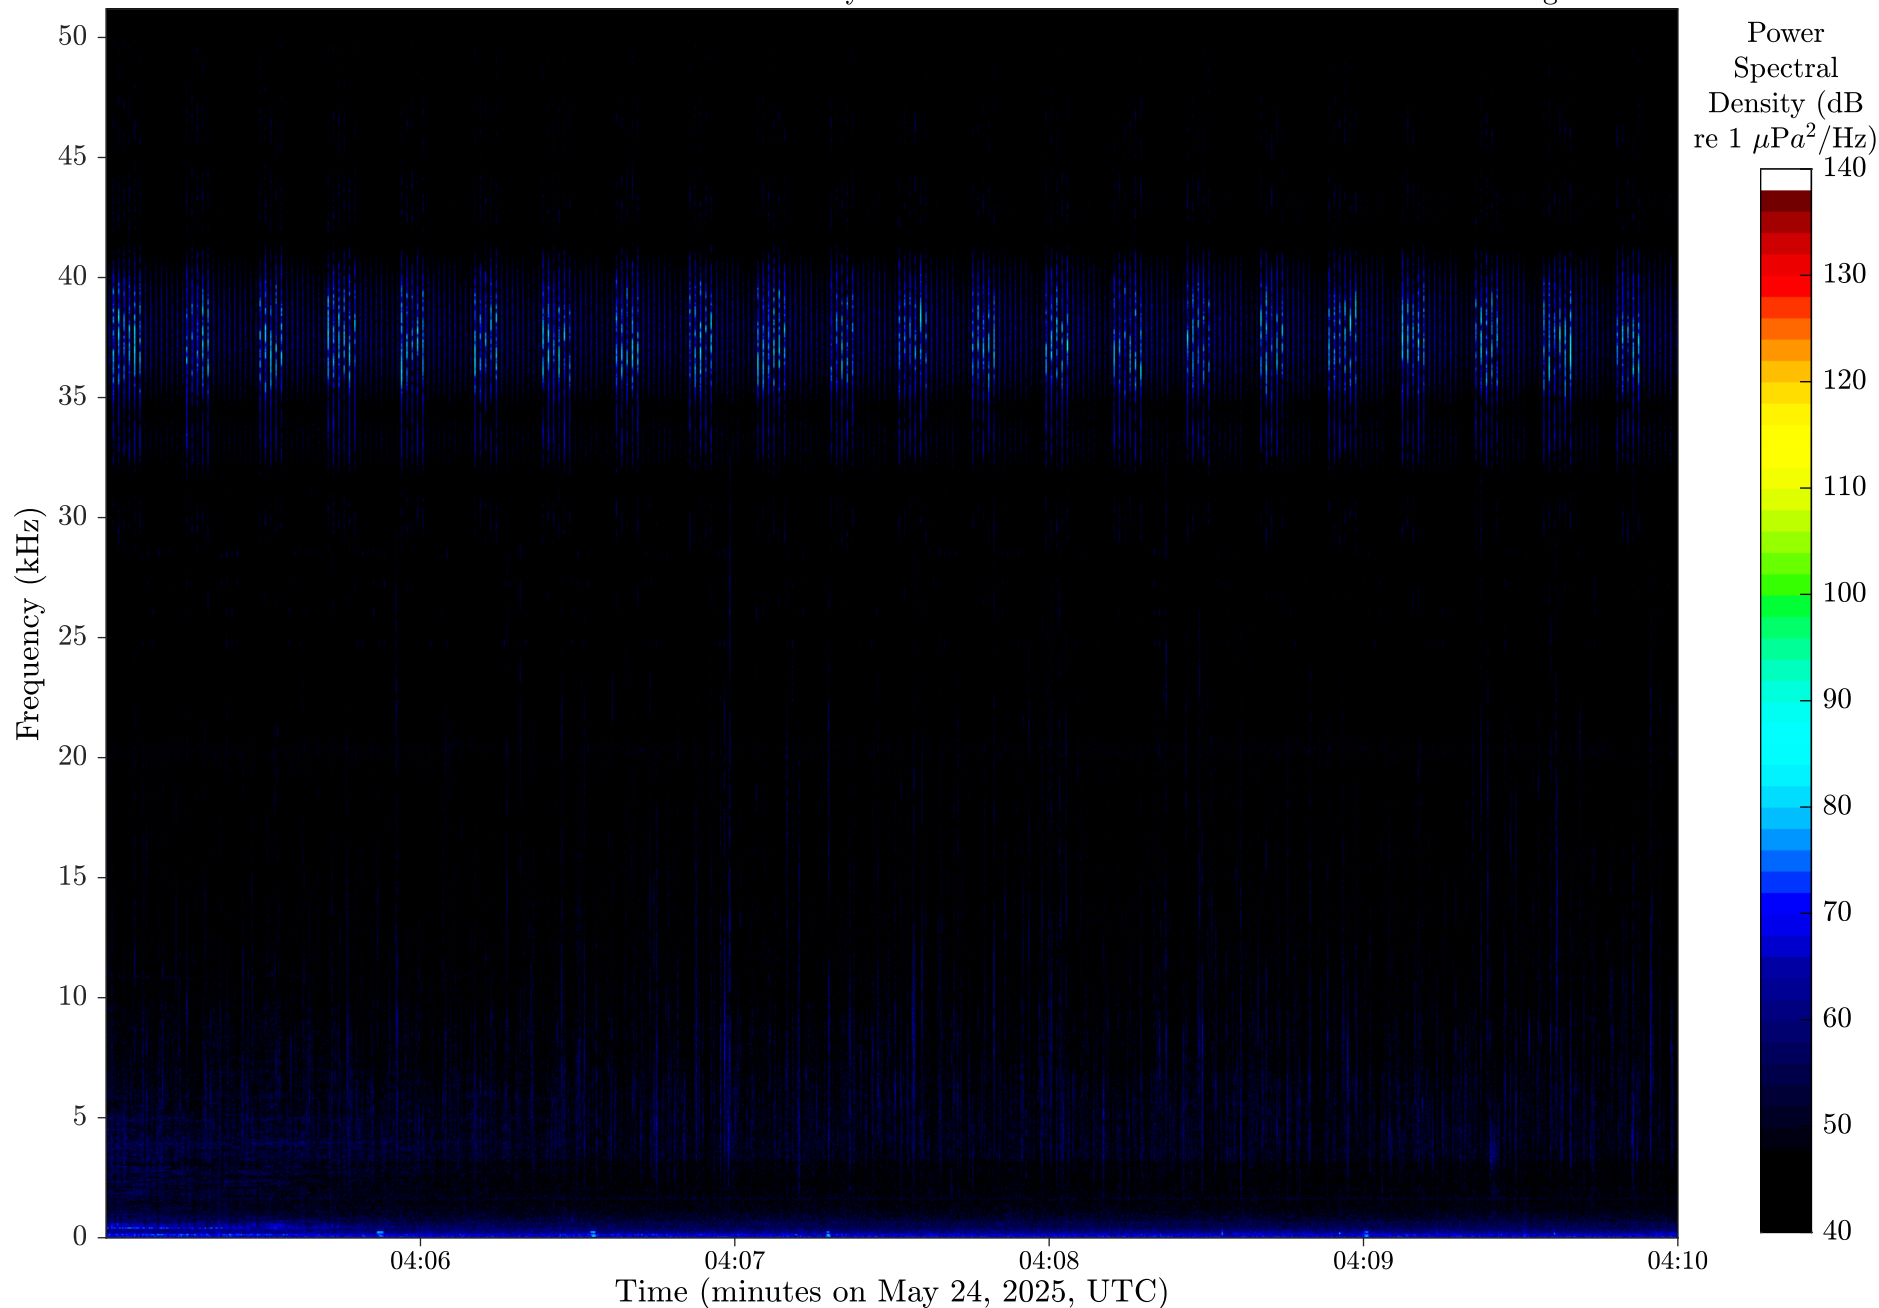


Comments: 34.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:25:49 UTC

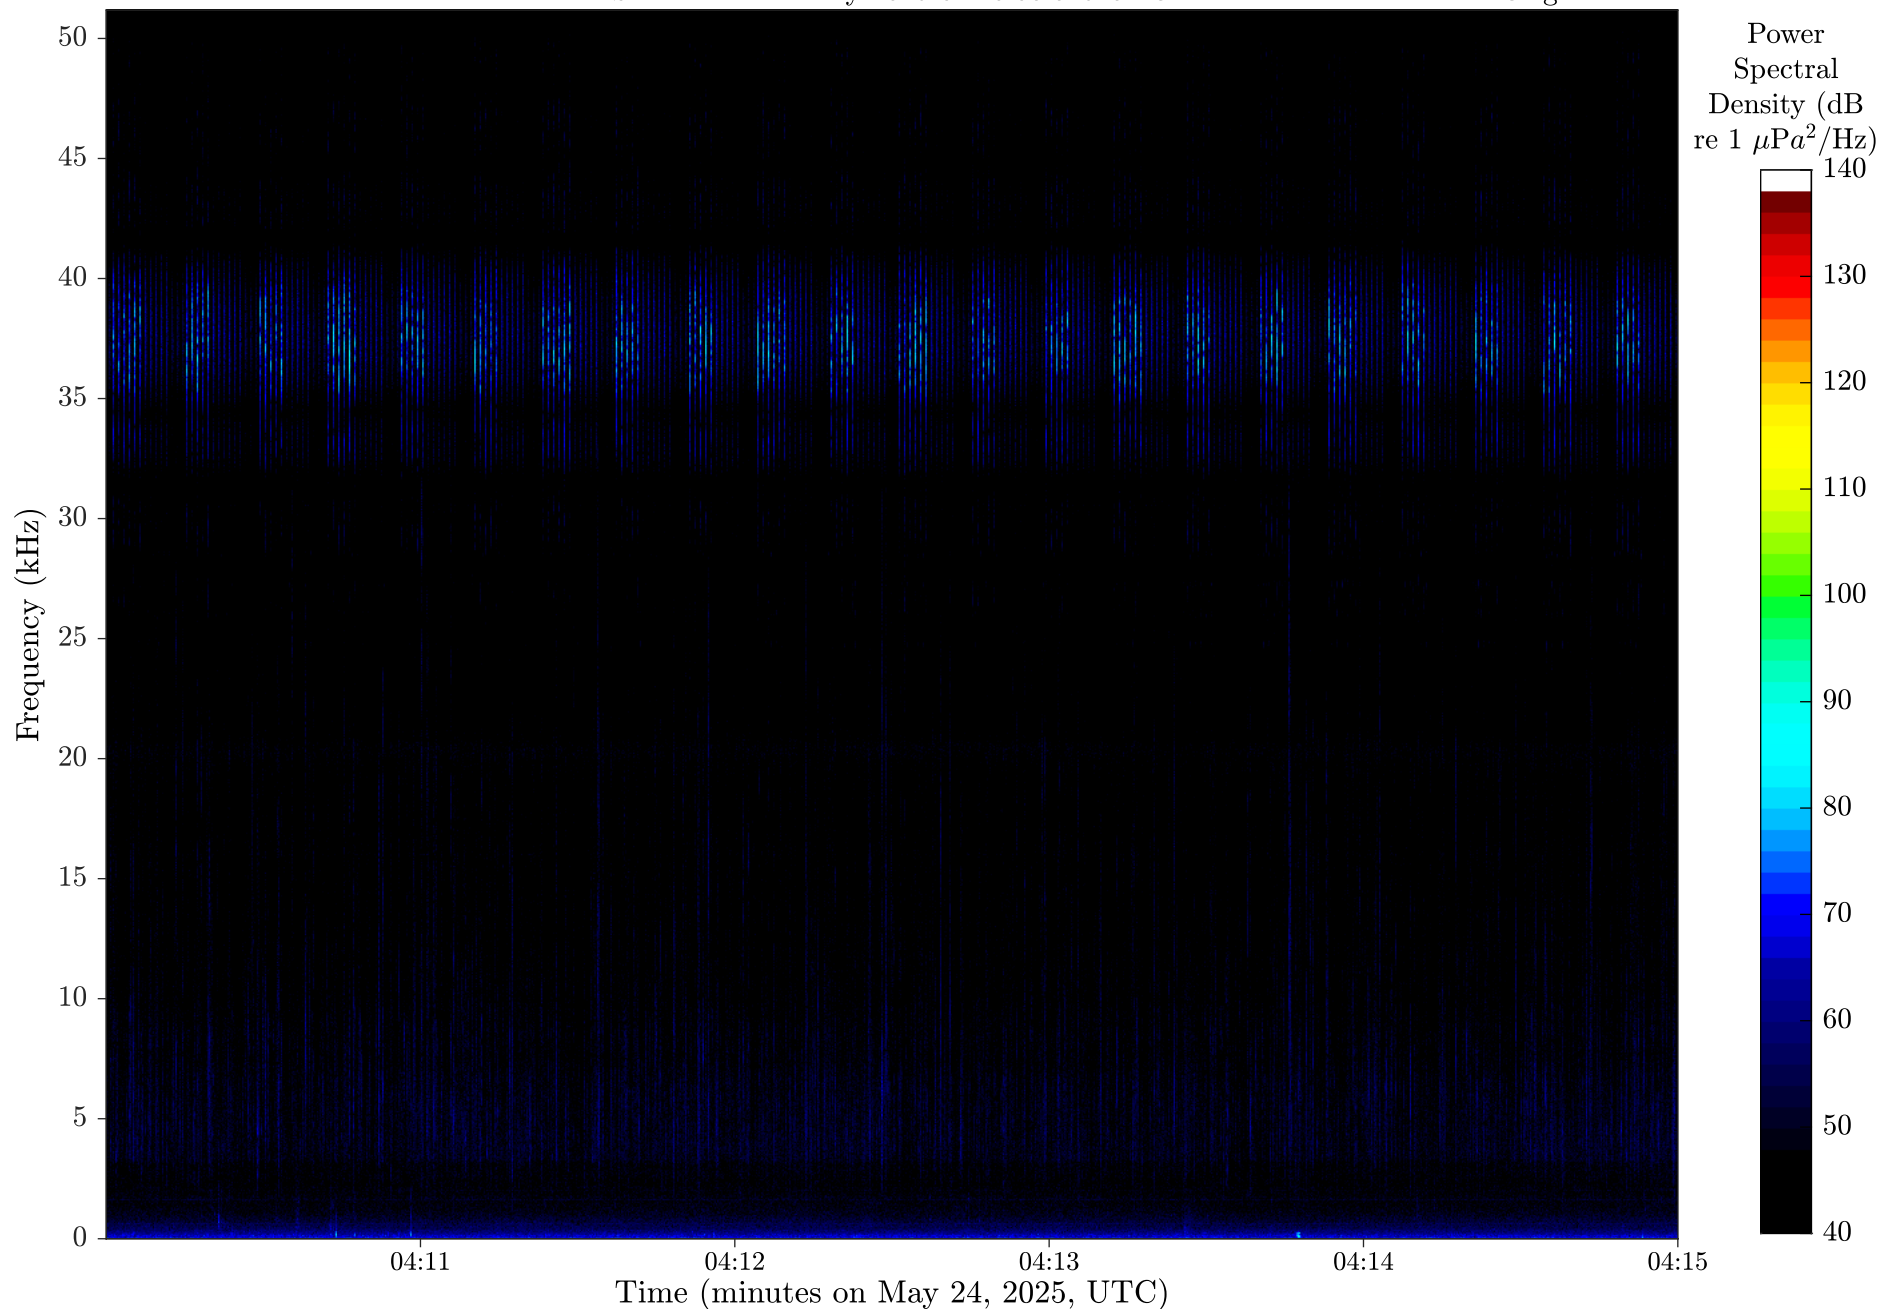


Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:25:58 UTC

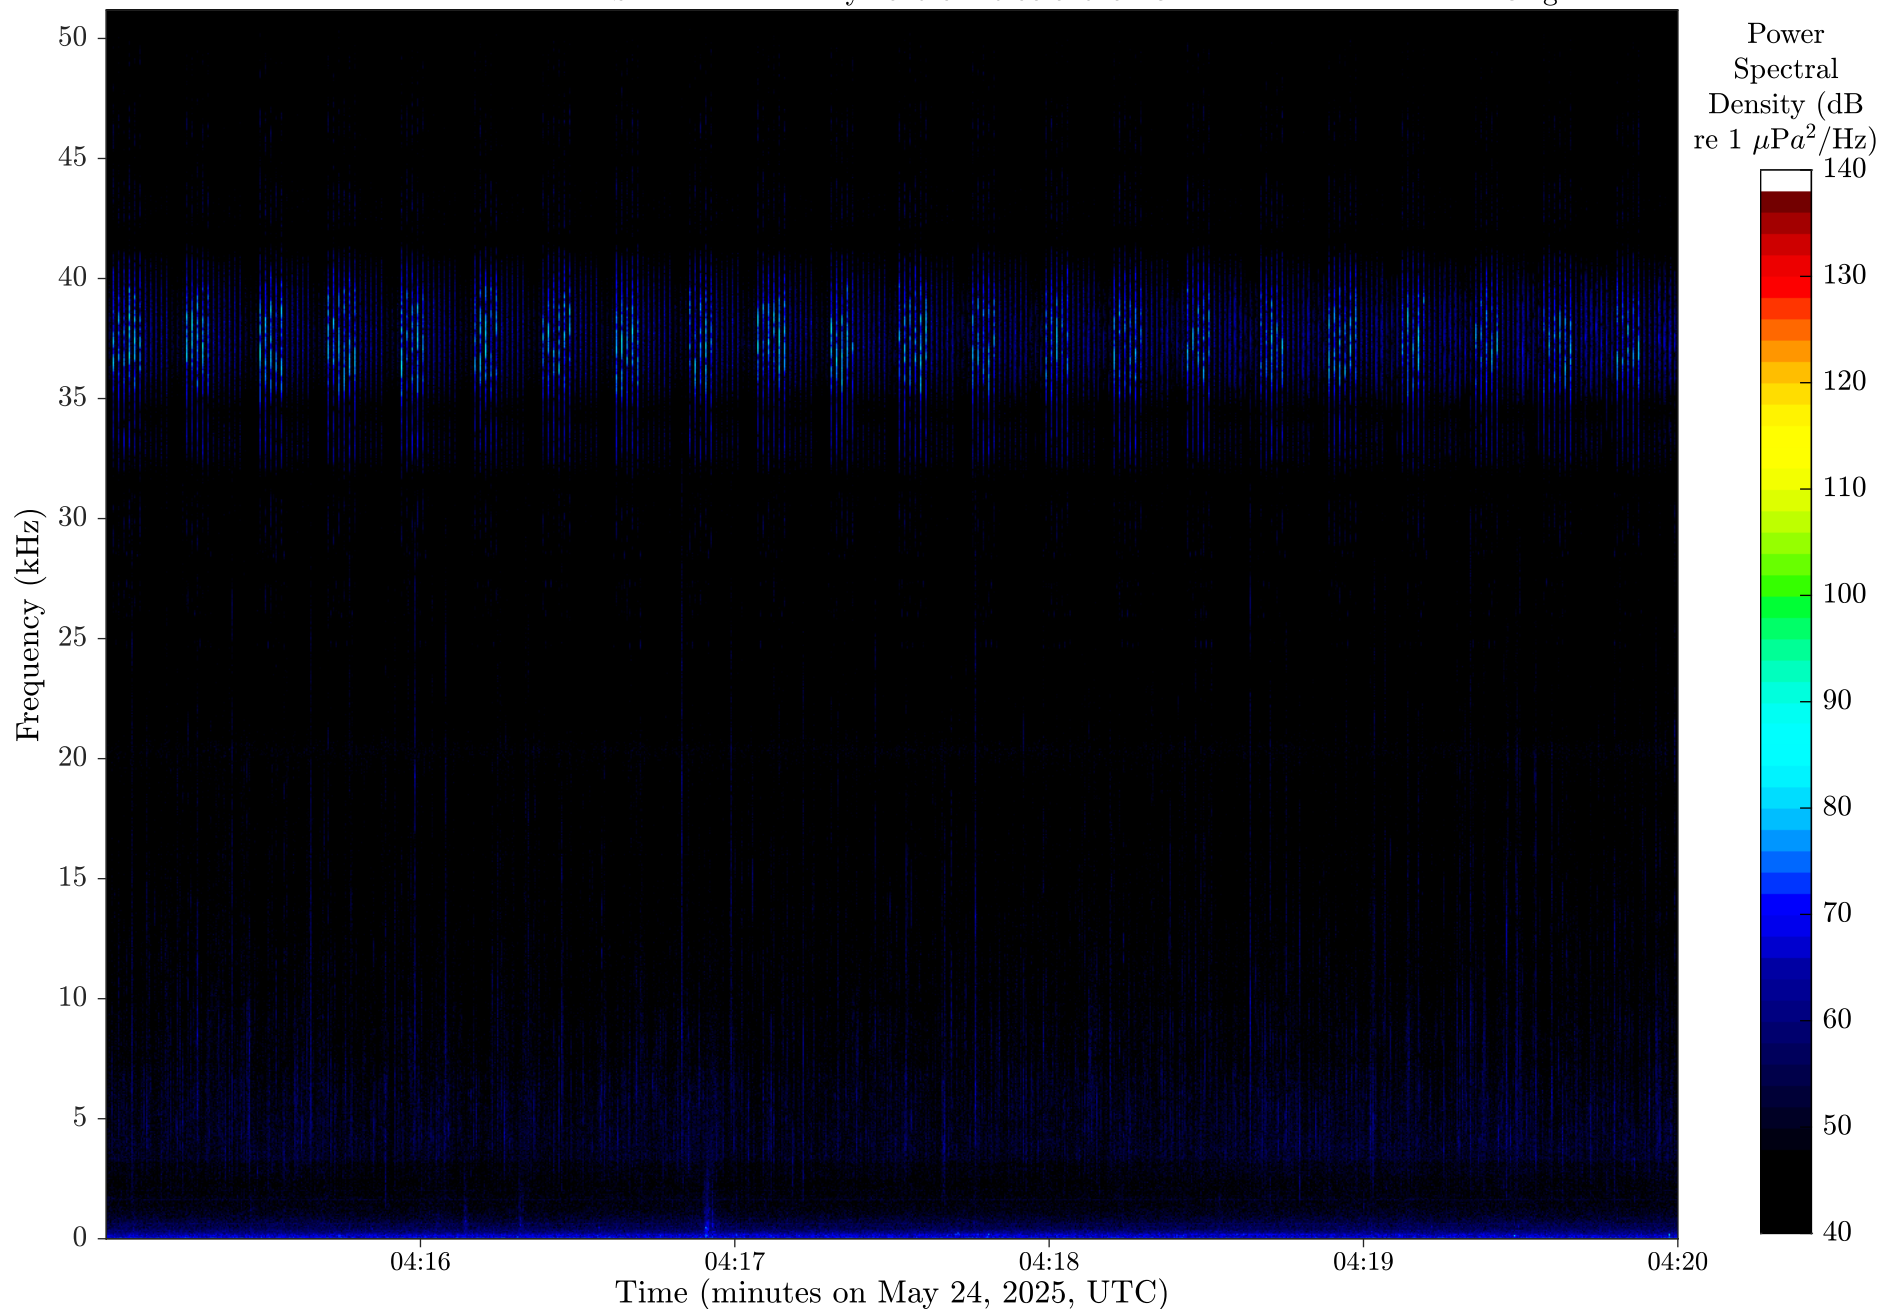

Comments: 34.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:26:06 UTC

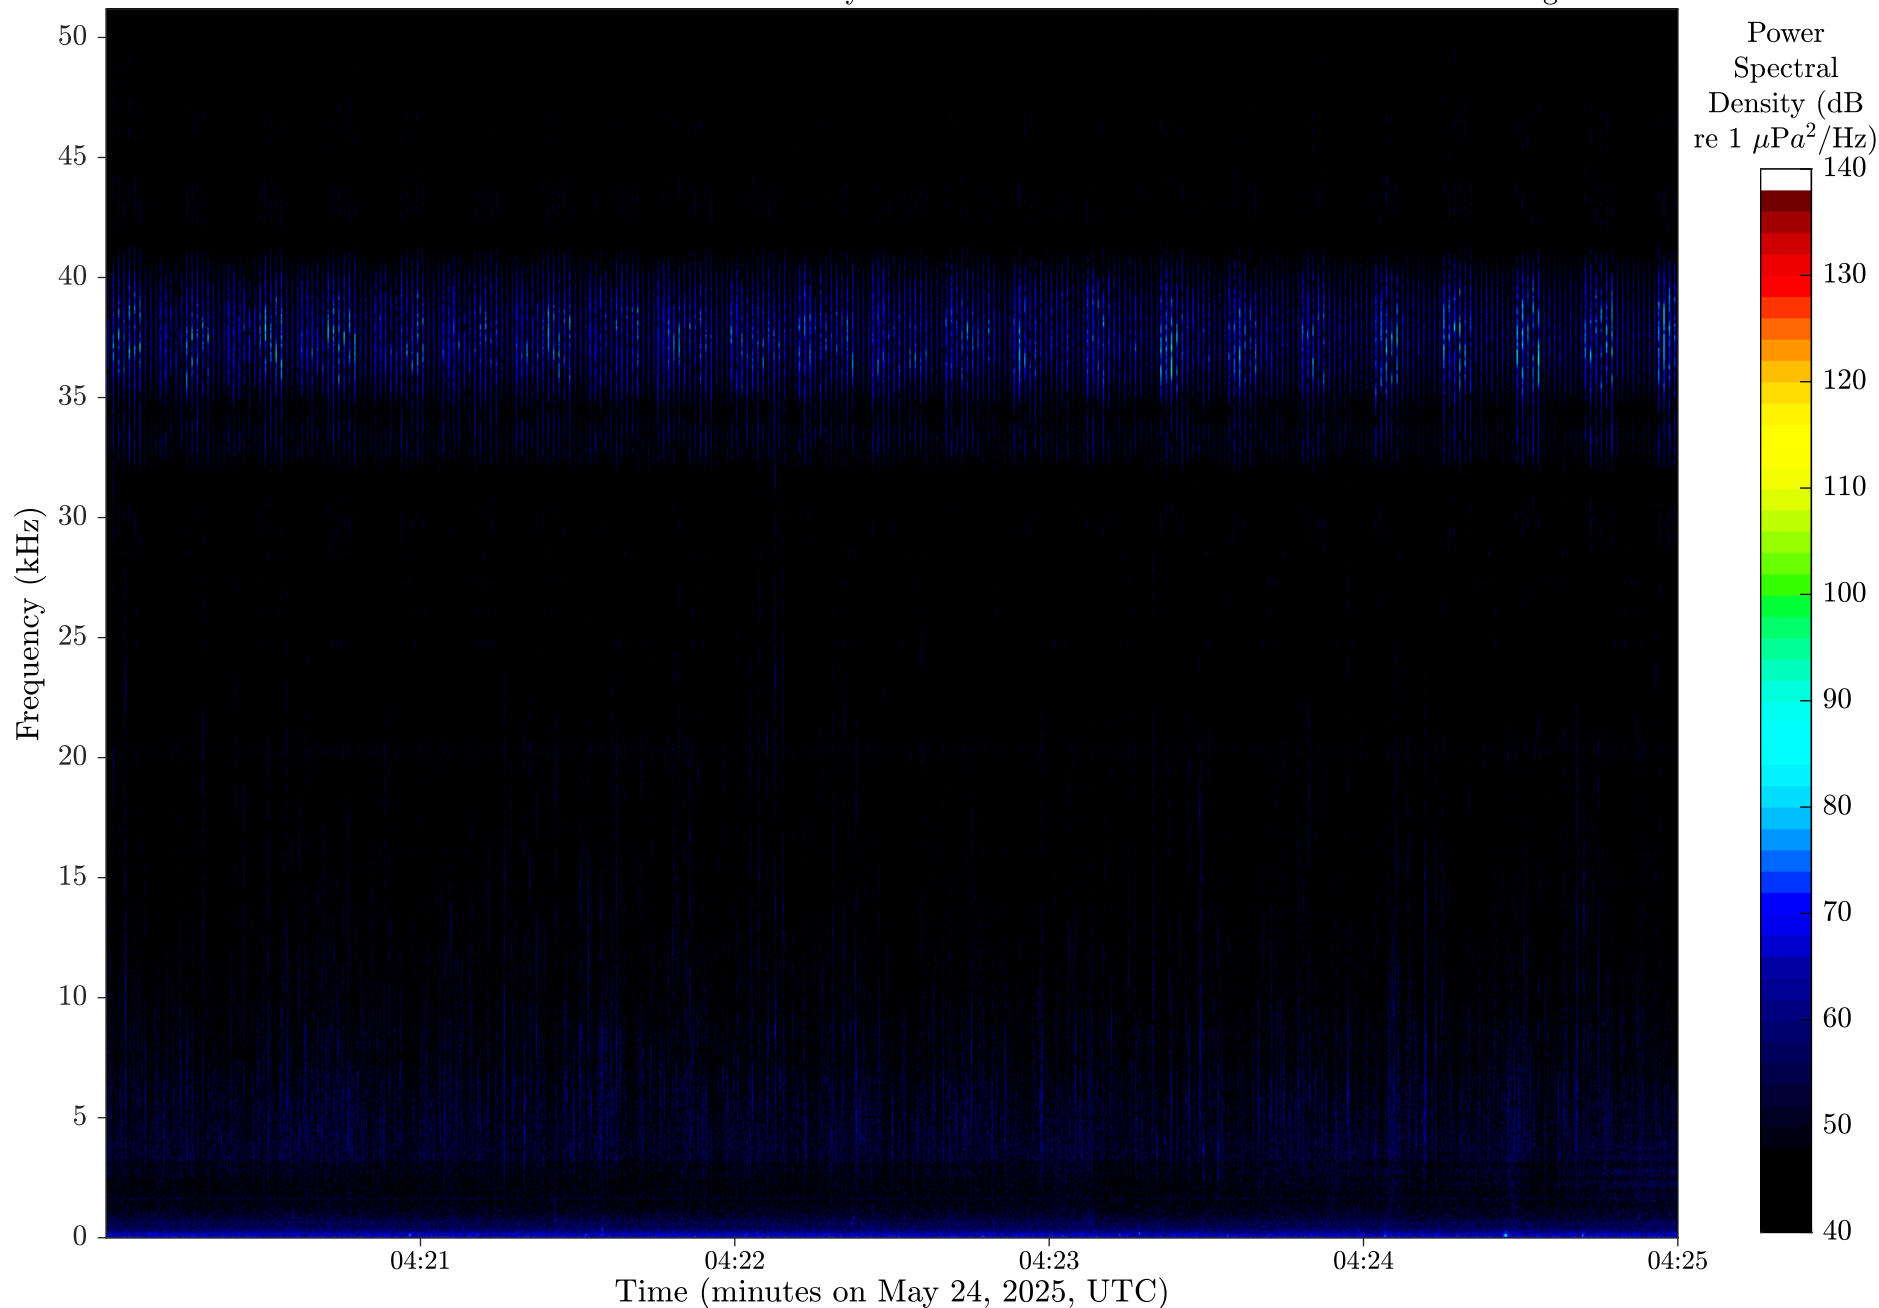

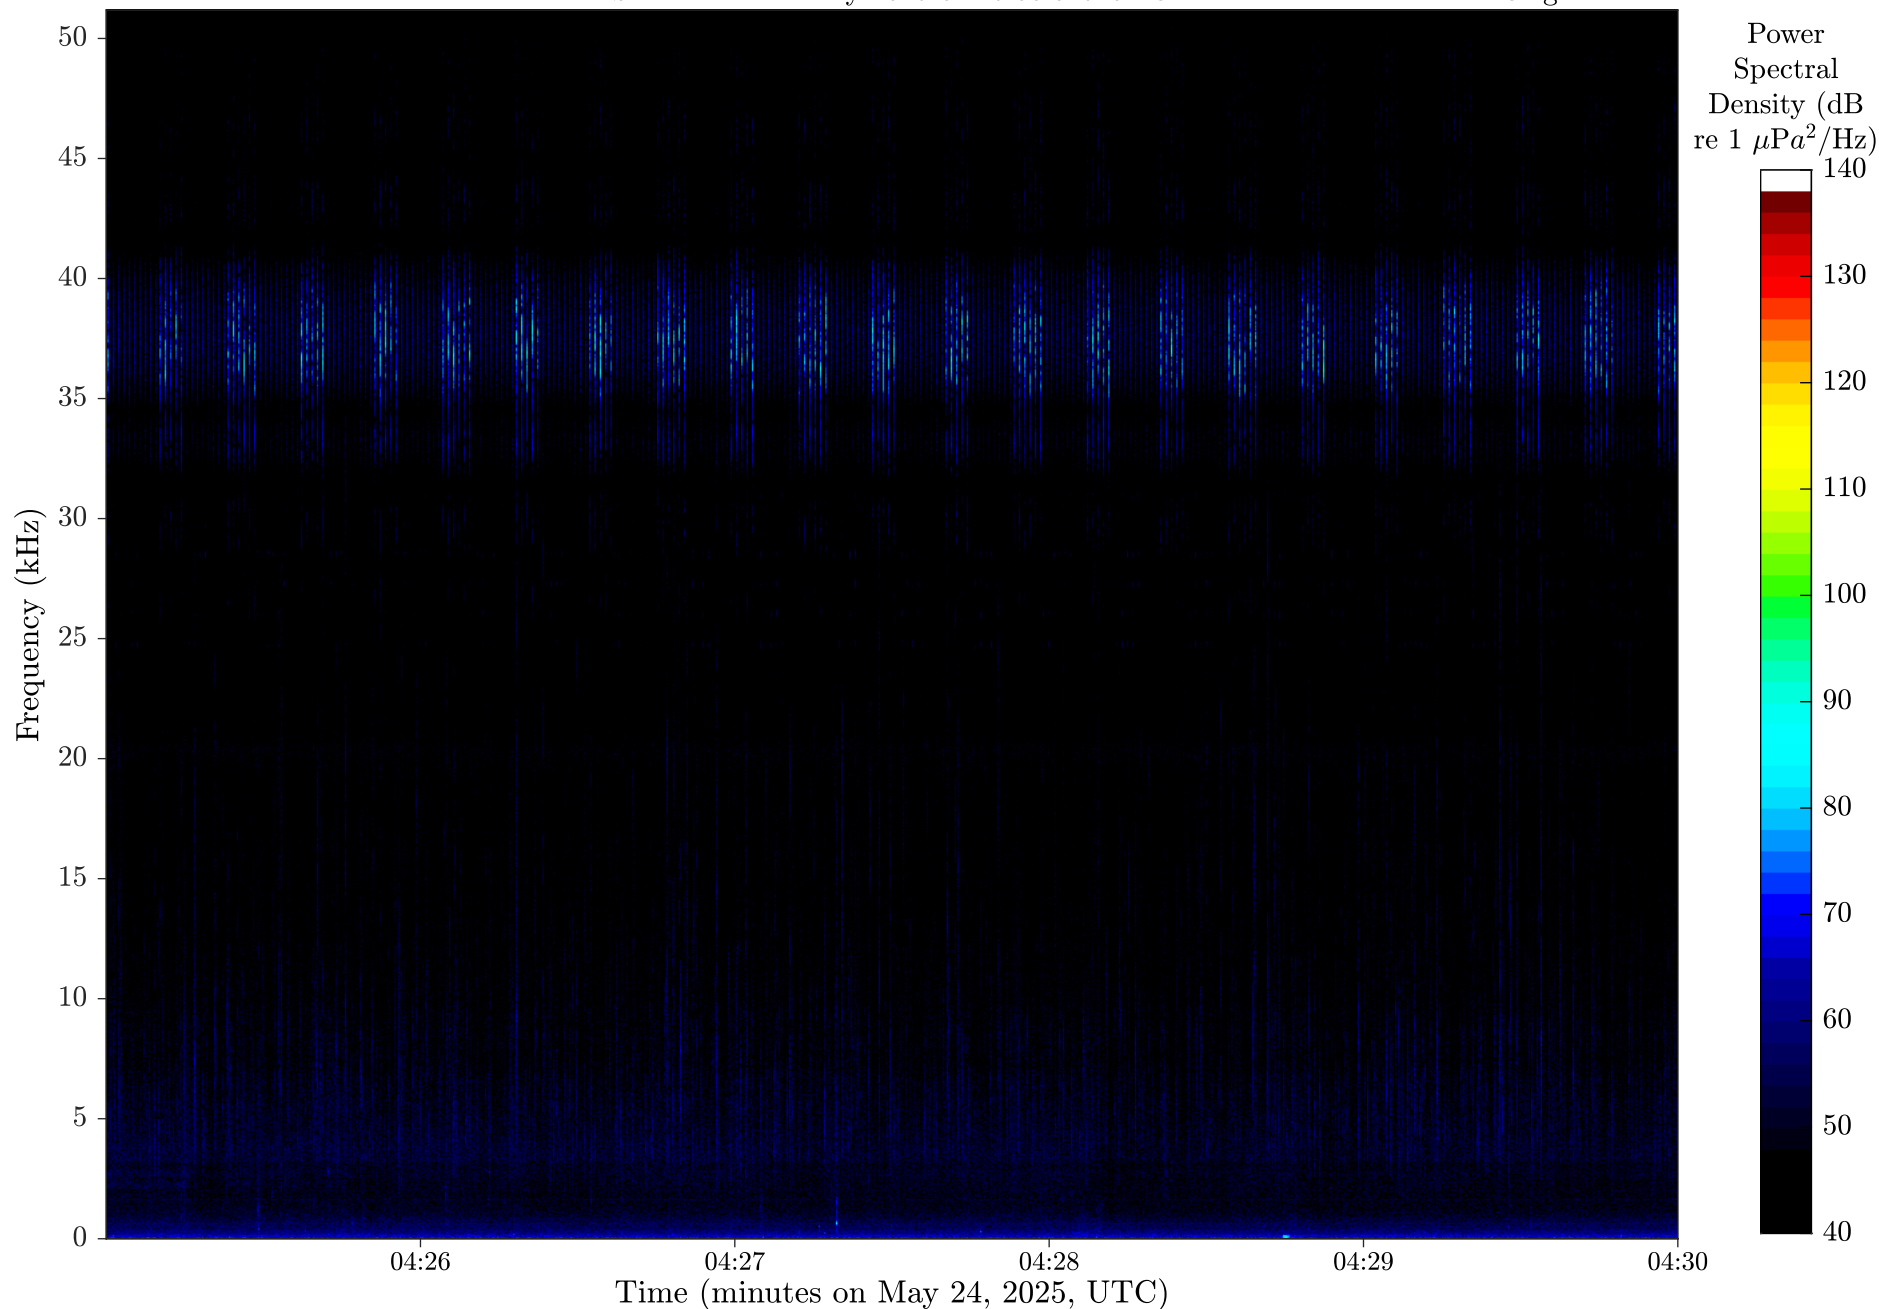


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:26:24 UTC

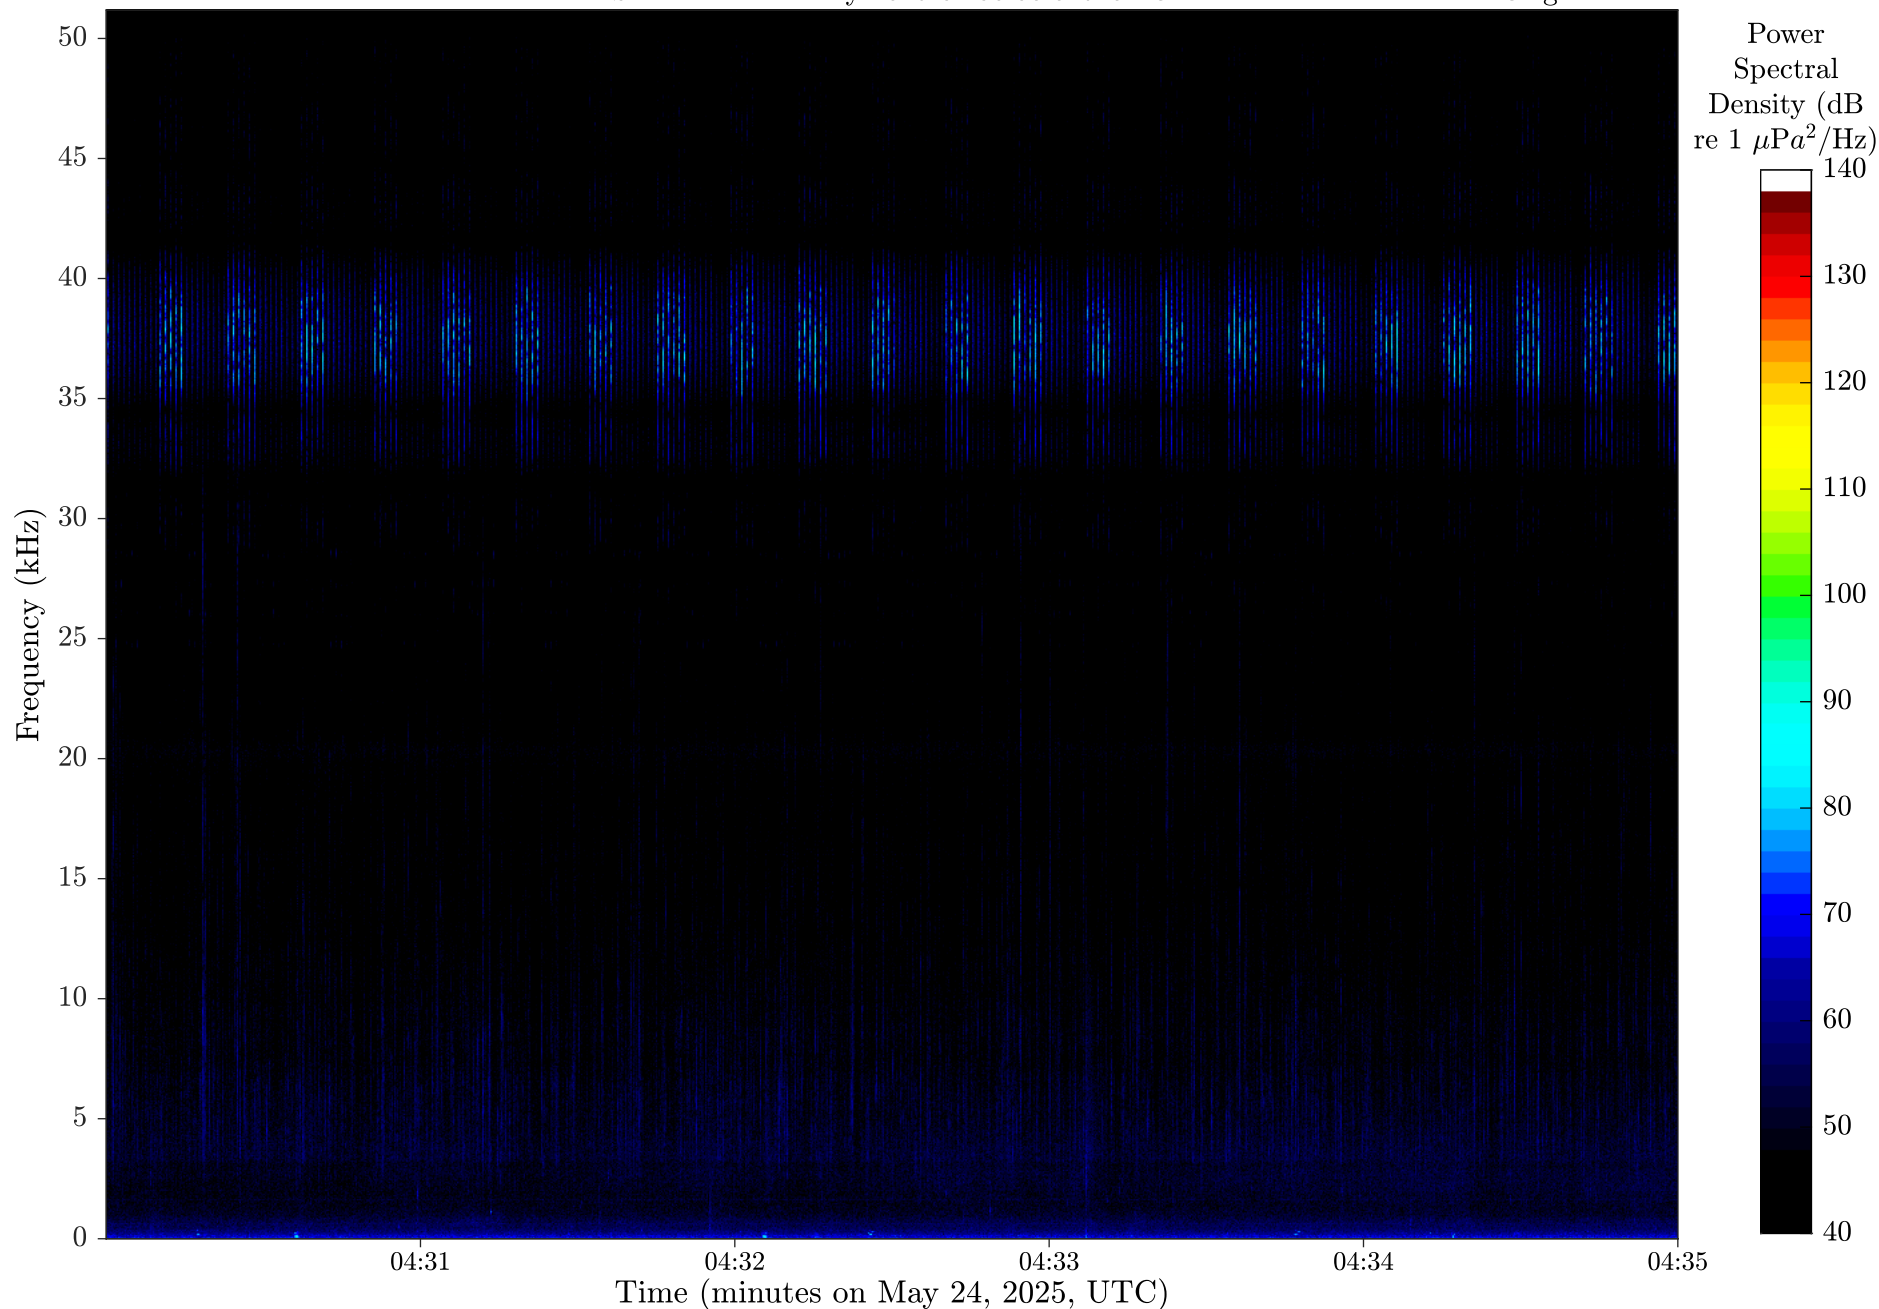


Comments: 34.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:26:33 UTC

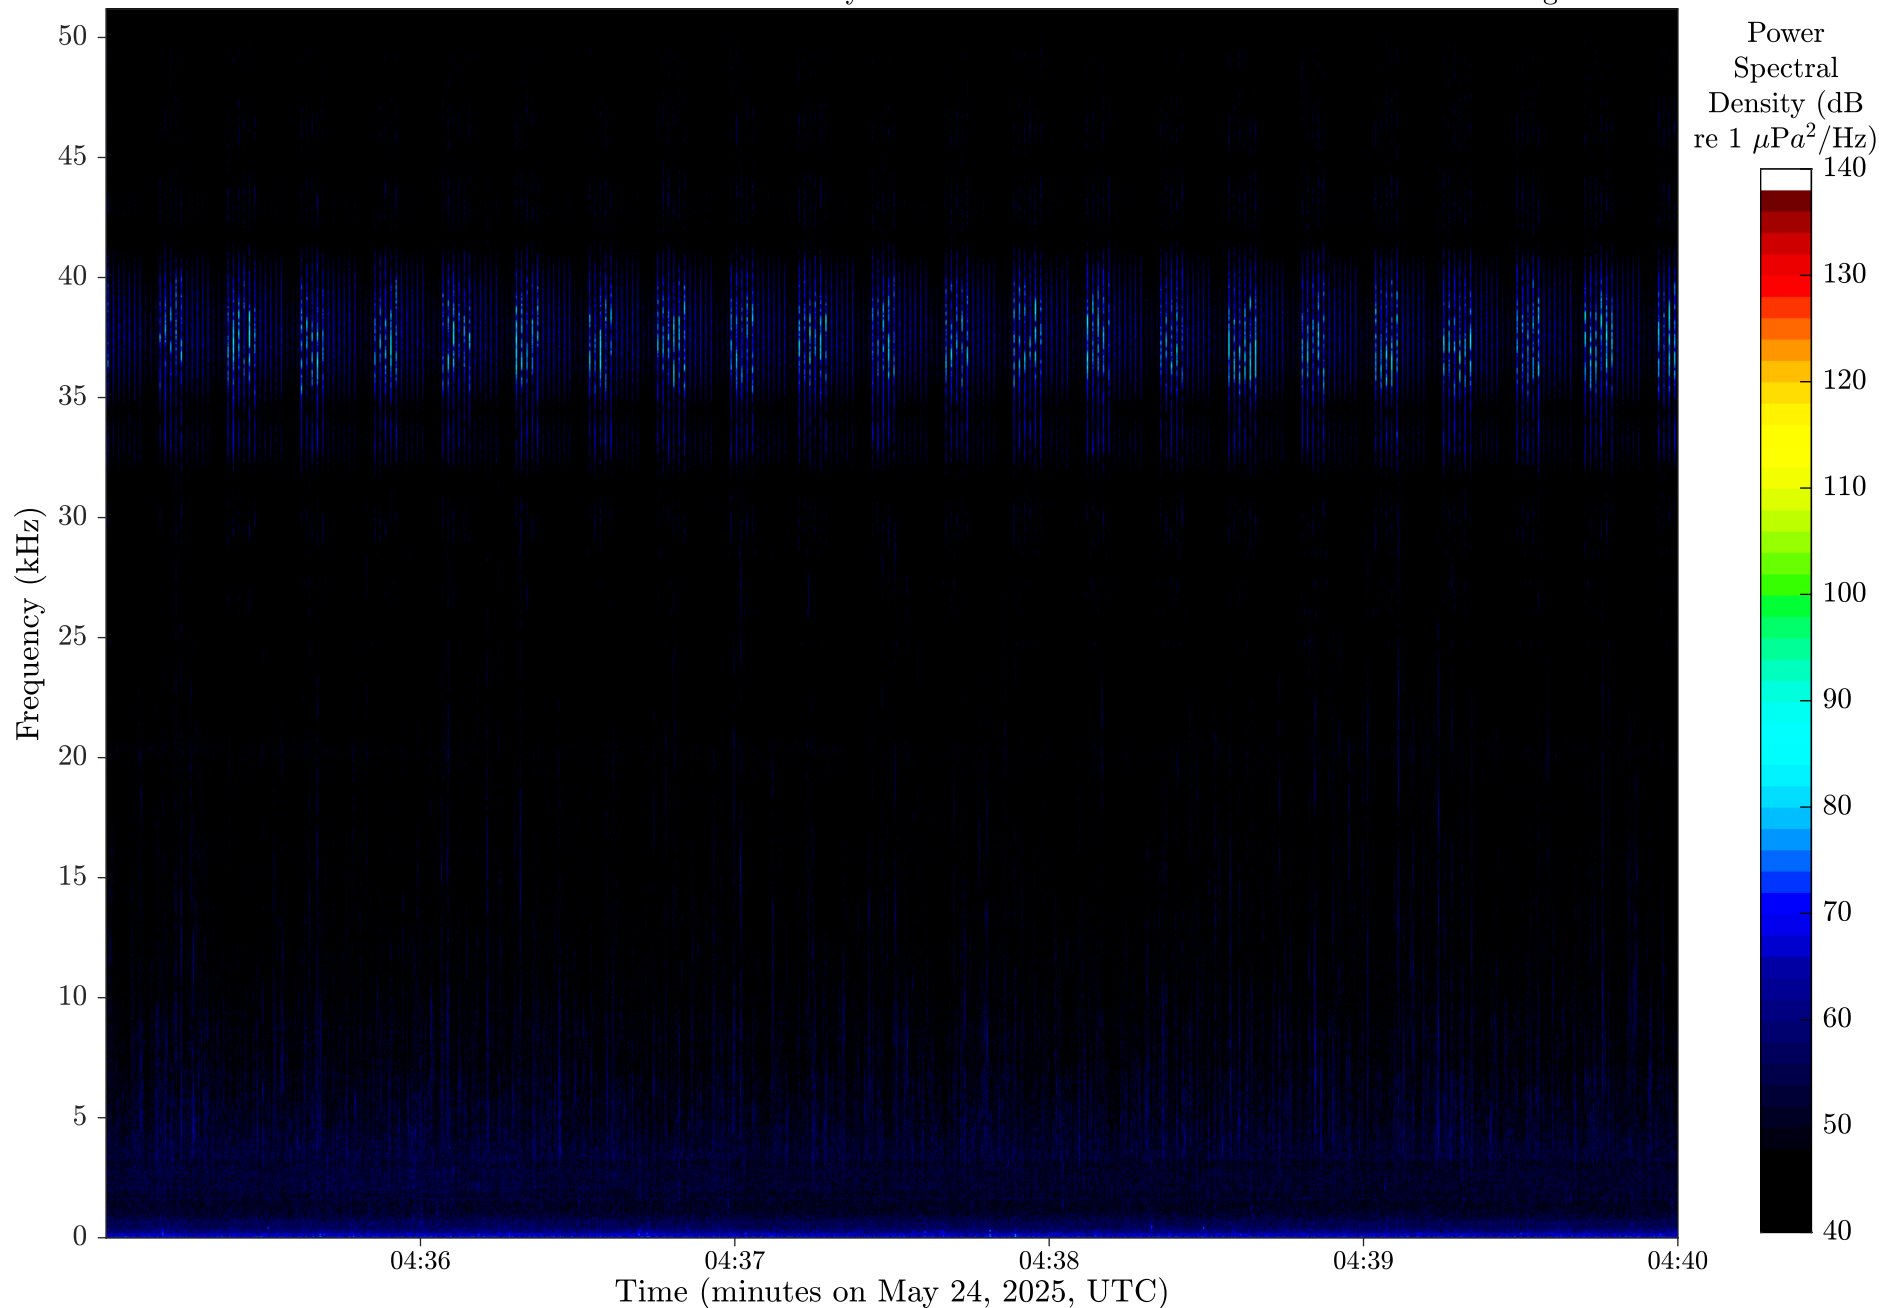


Comments: 34.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:26:41 UTC

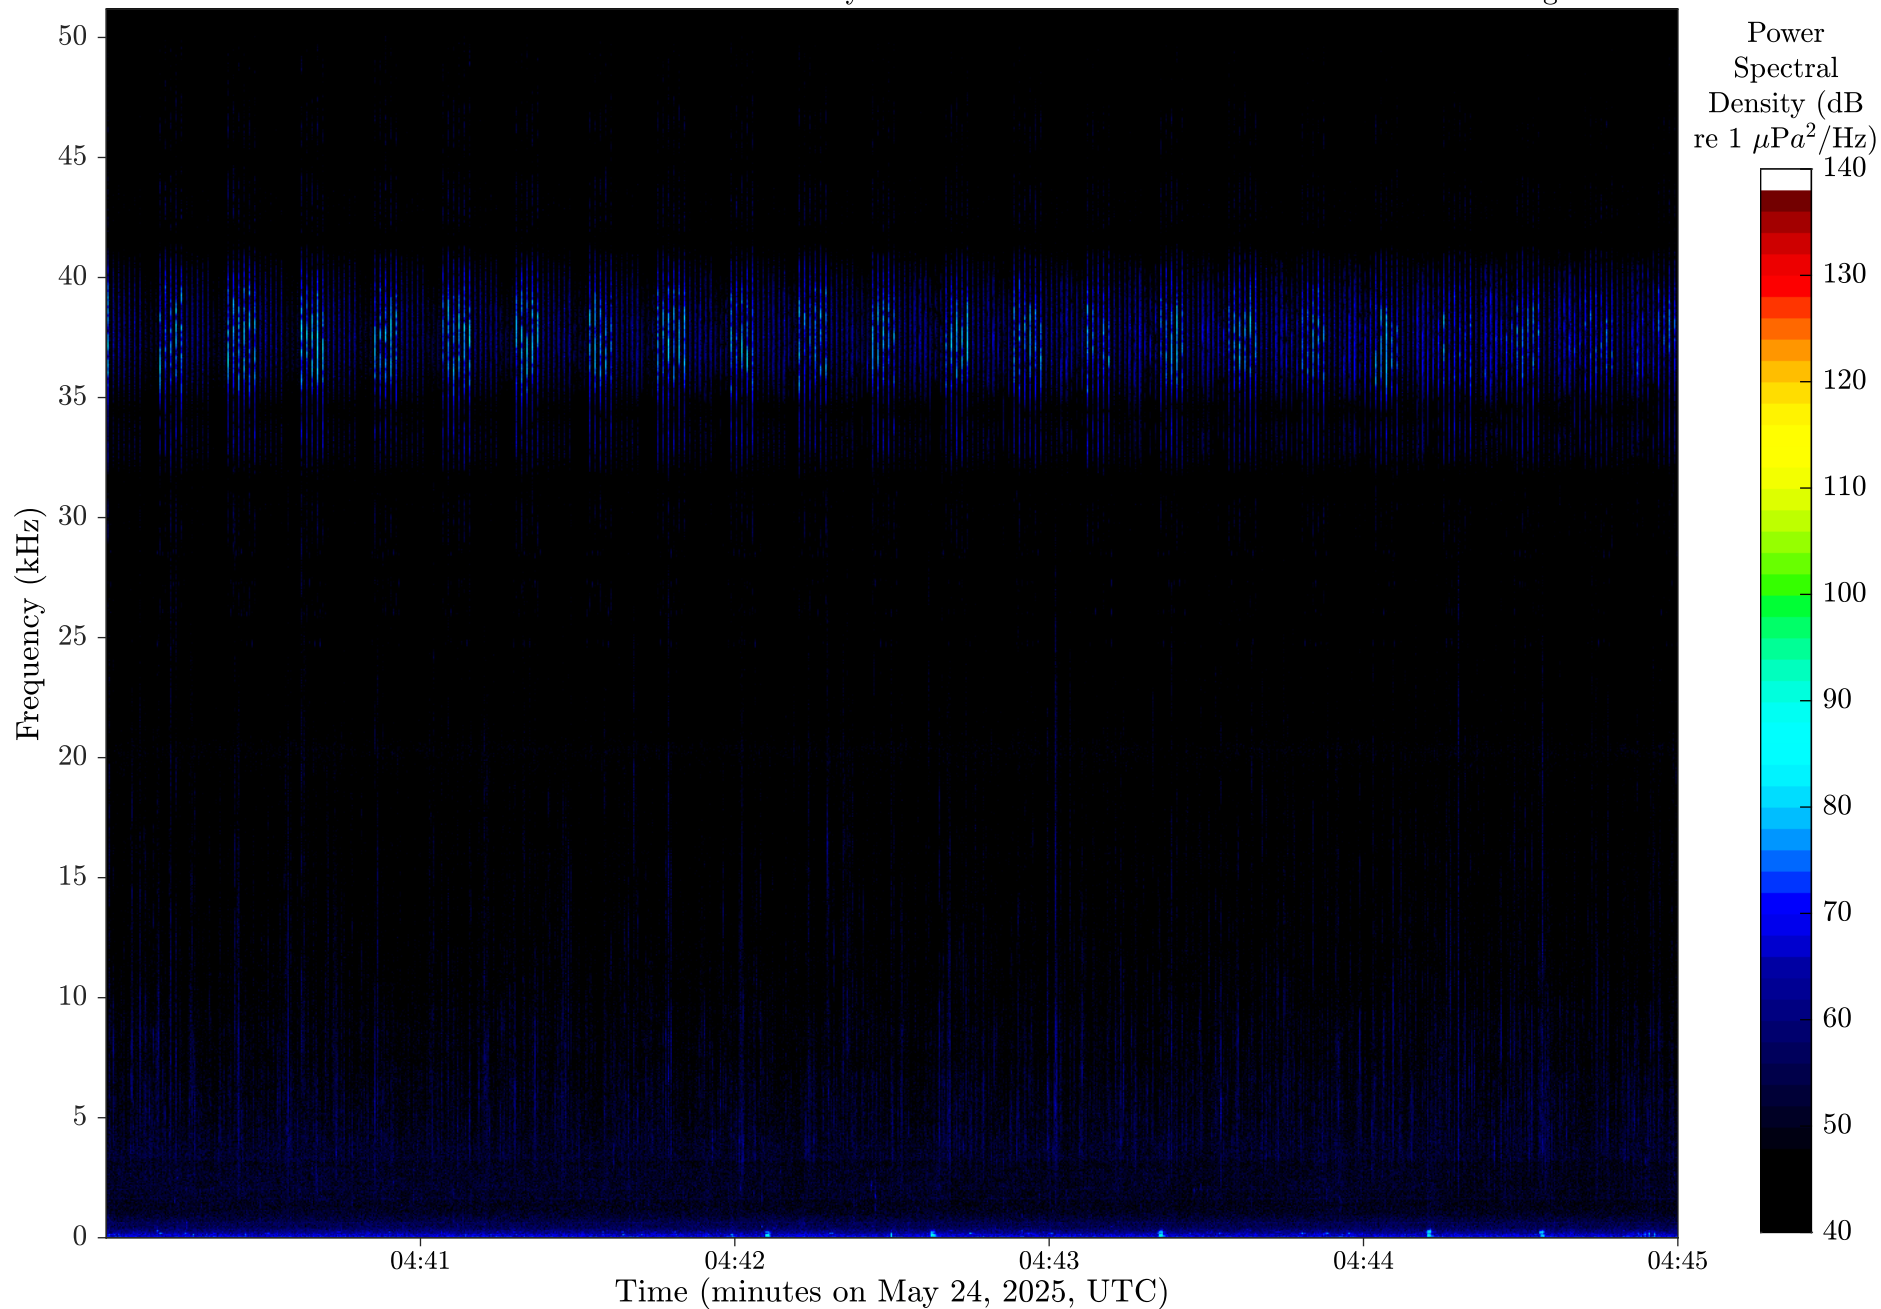


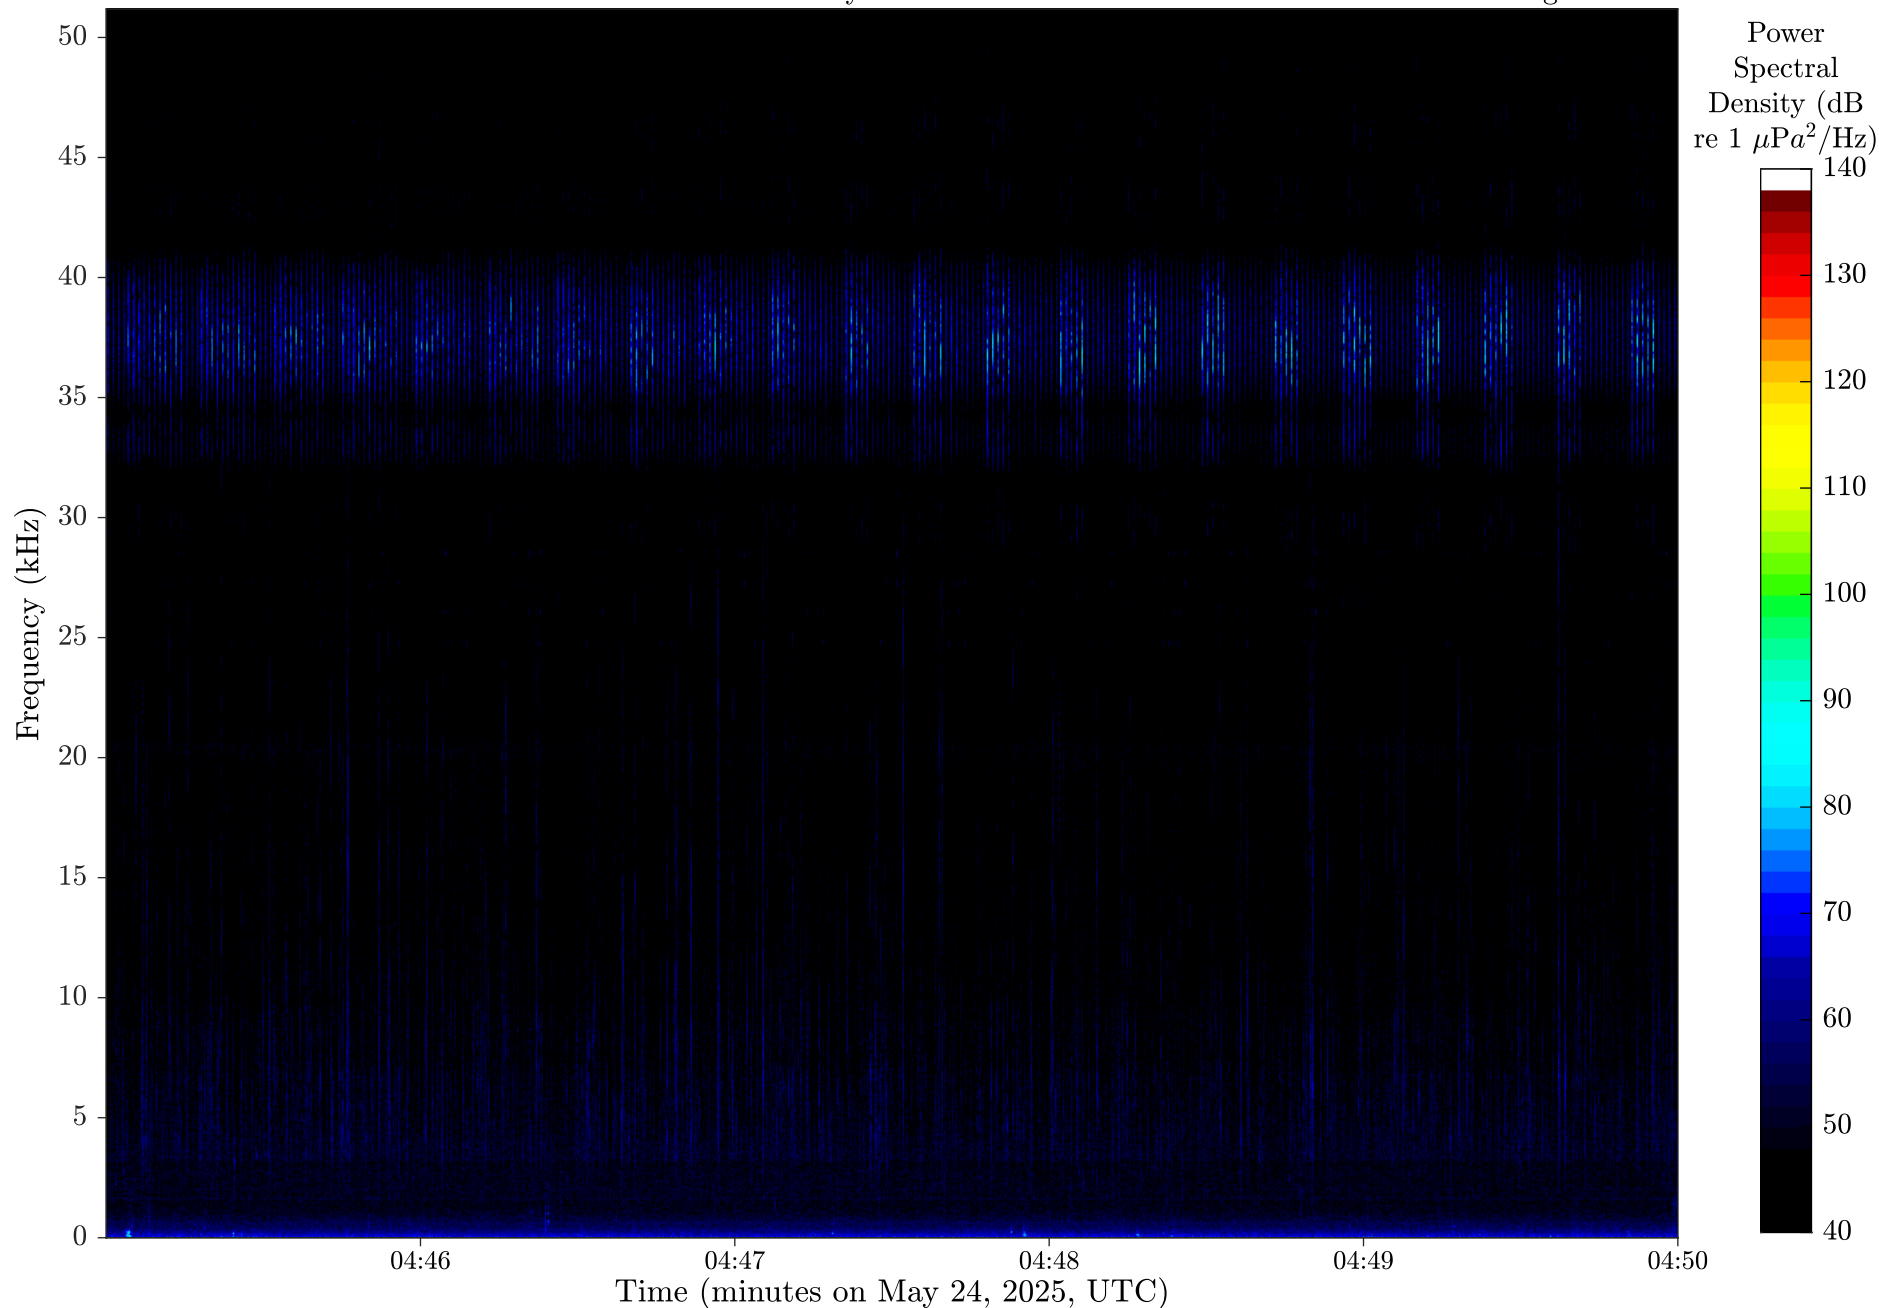

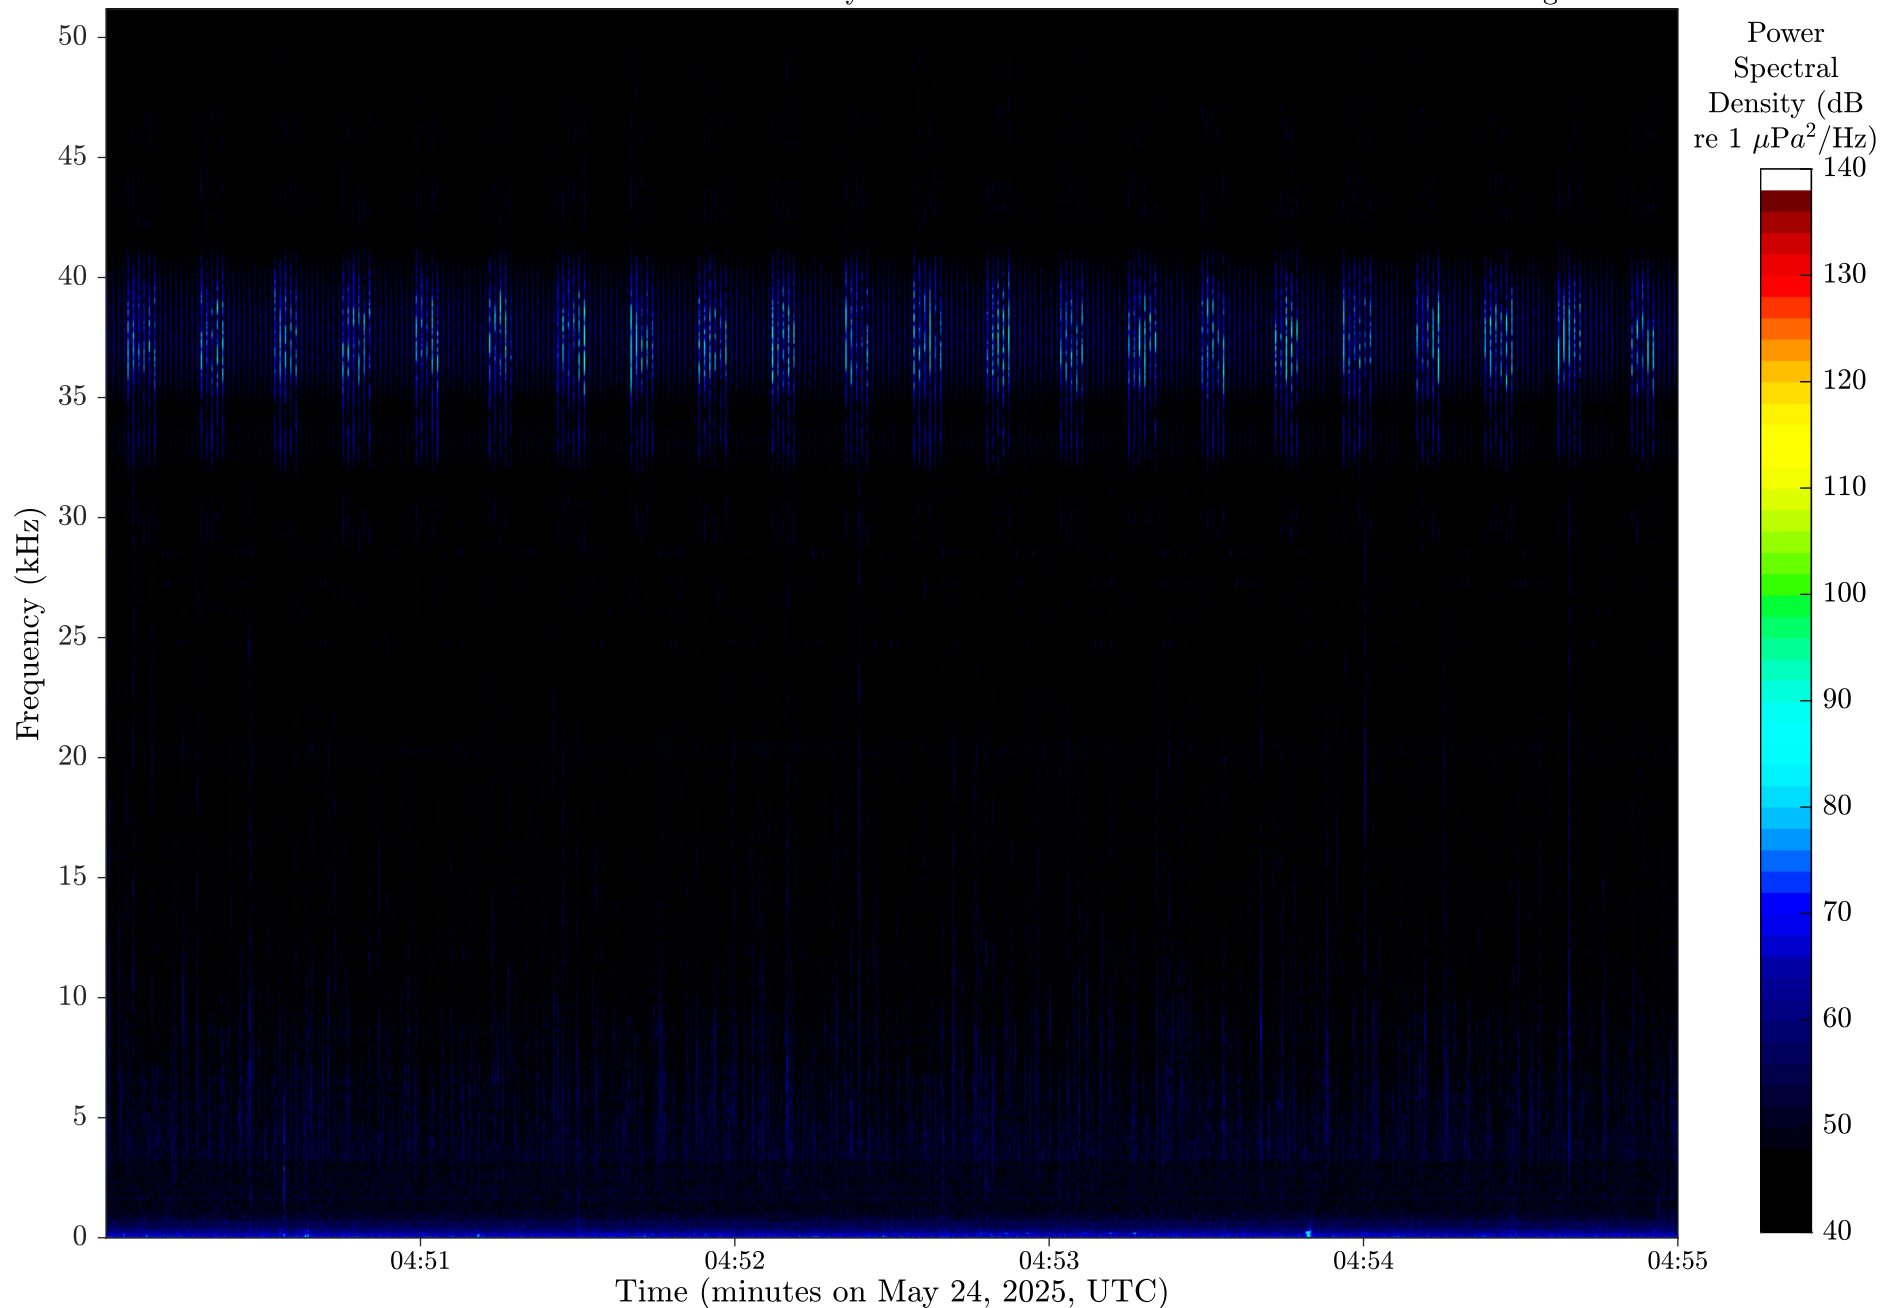


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:27:05 UTC

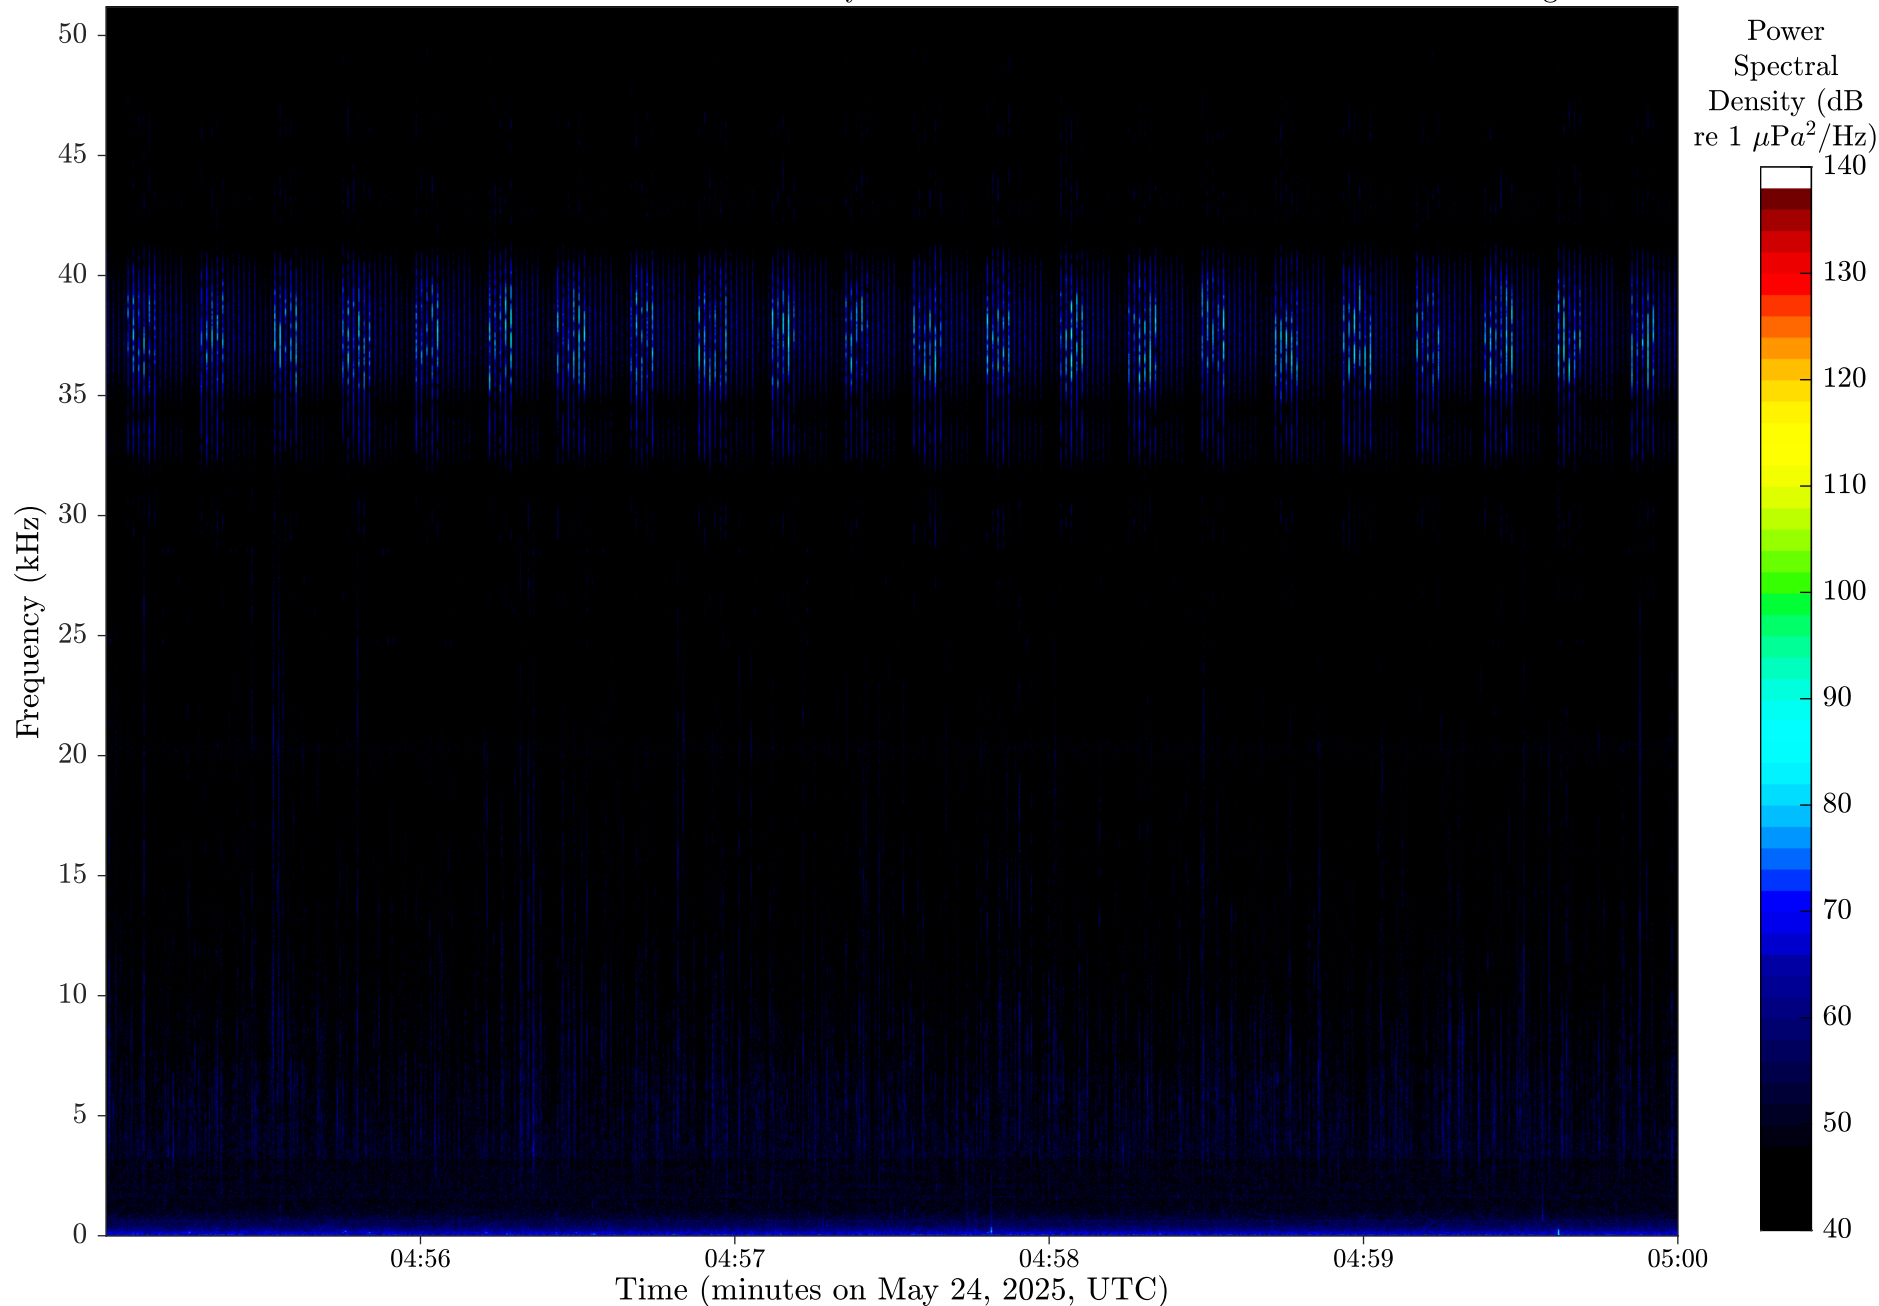


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:27:15 UTC

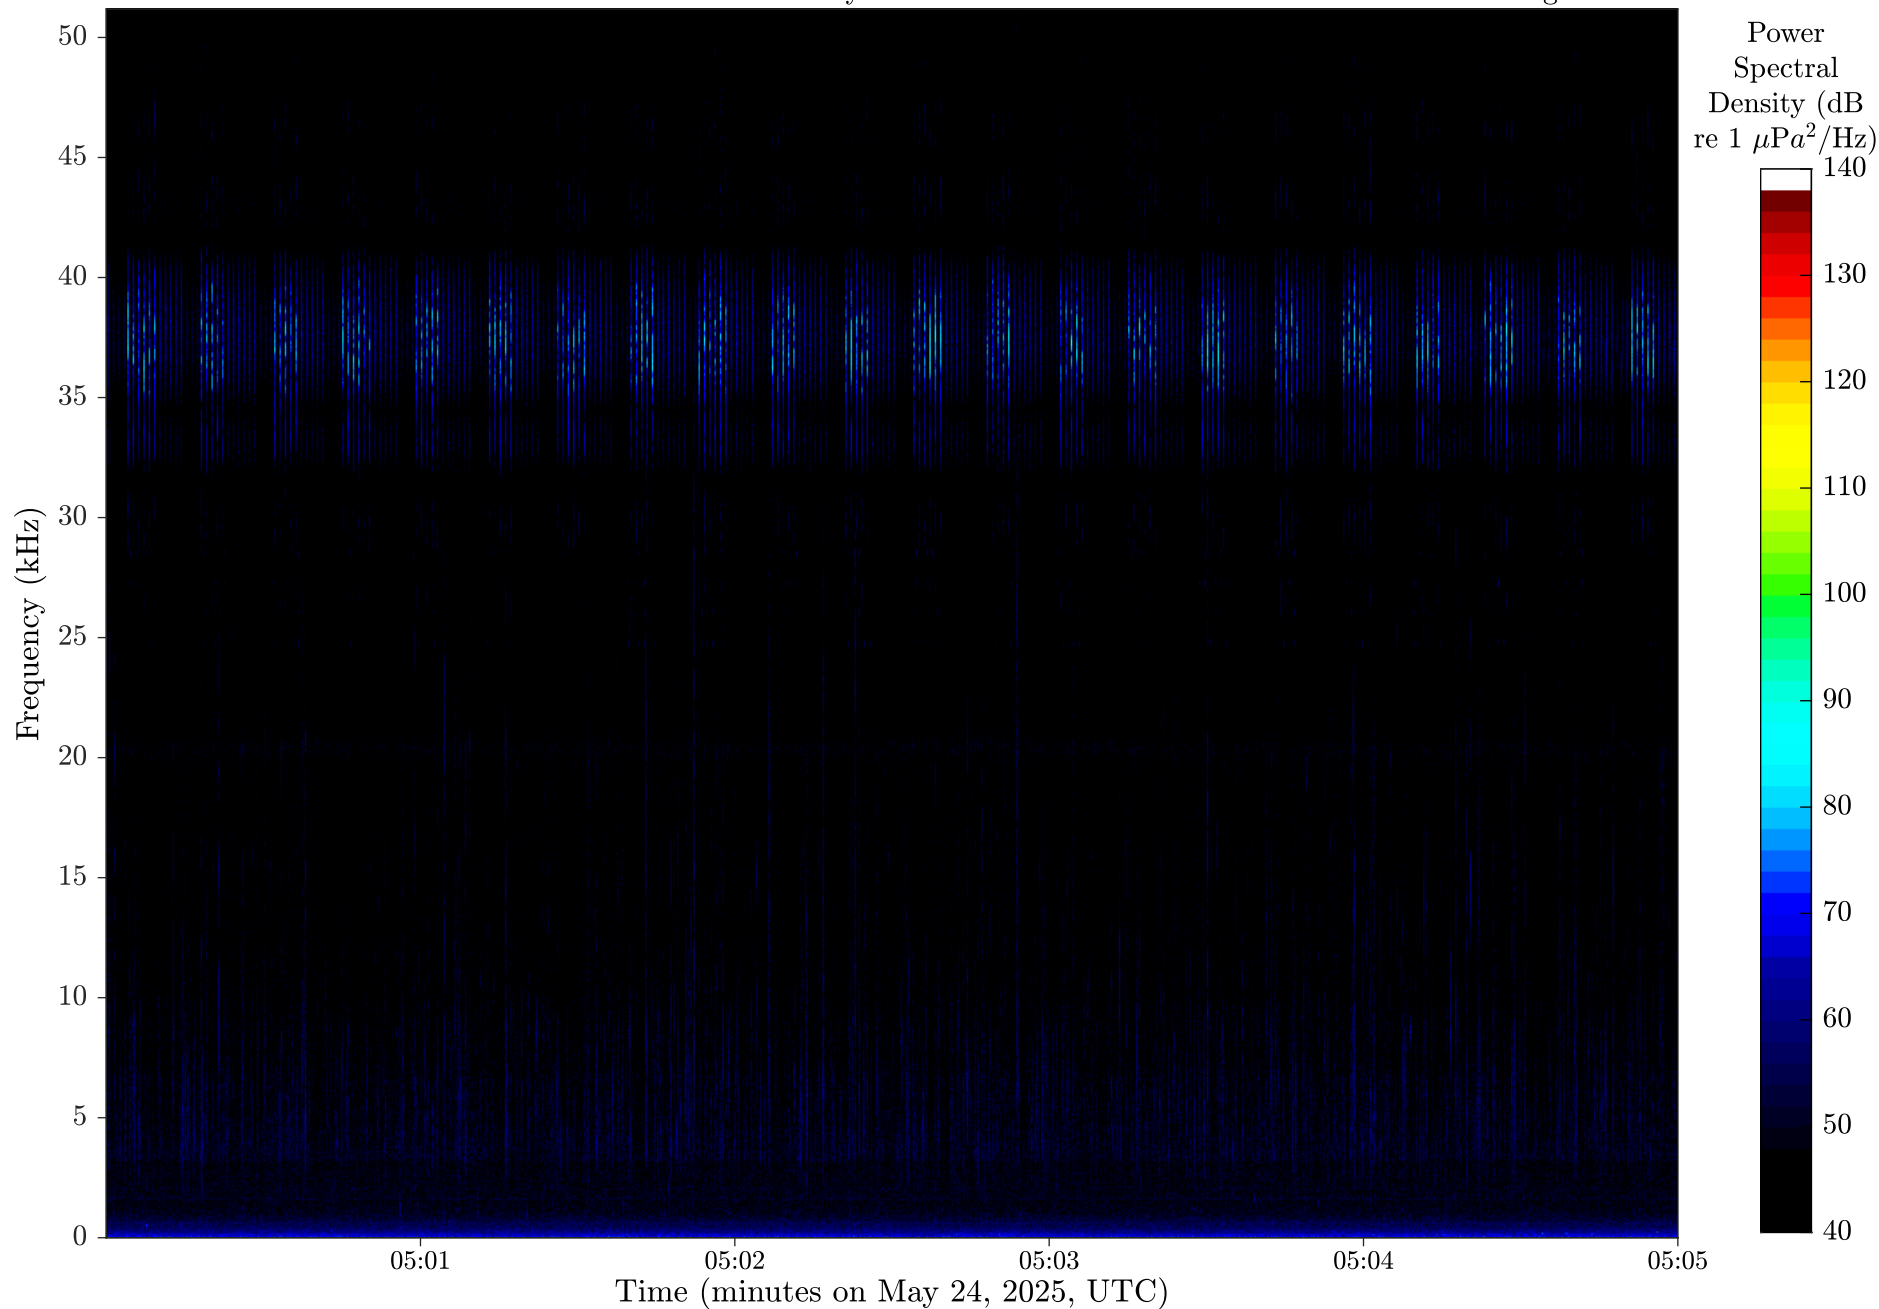


Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:27:24 UTC

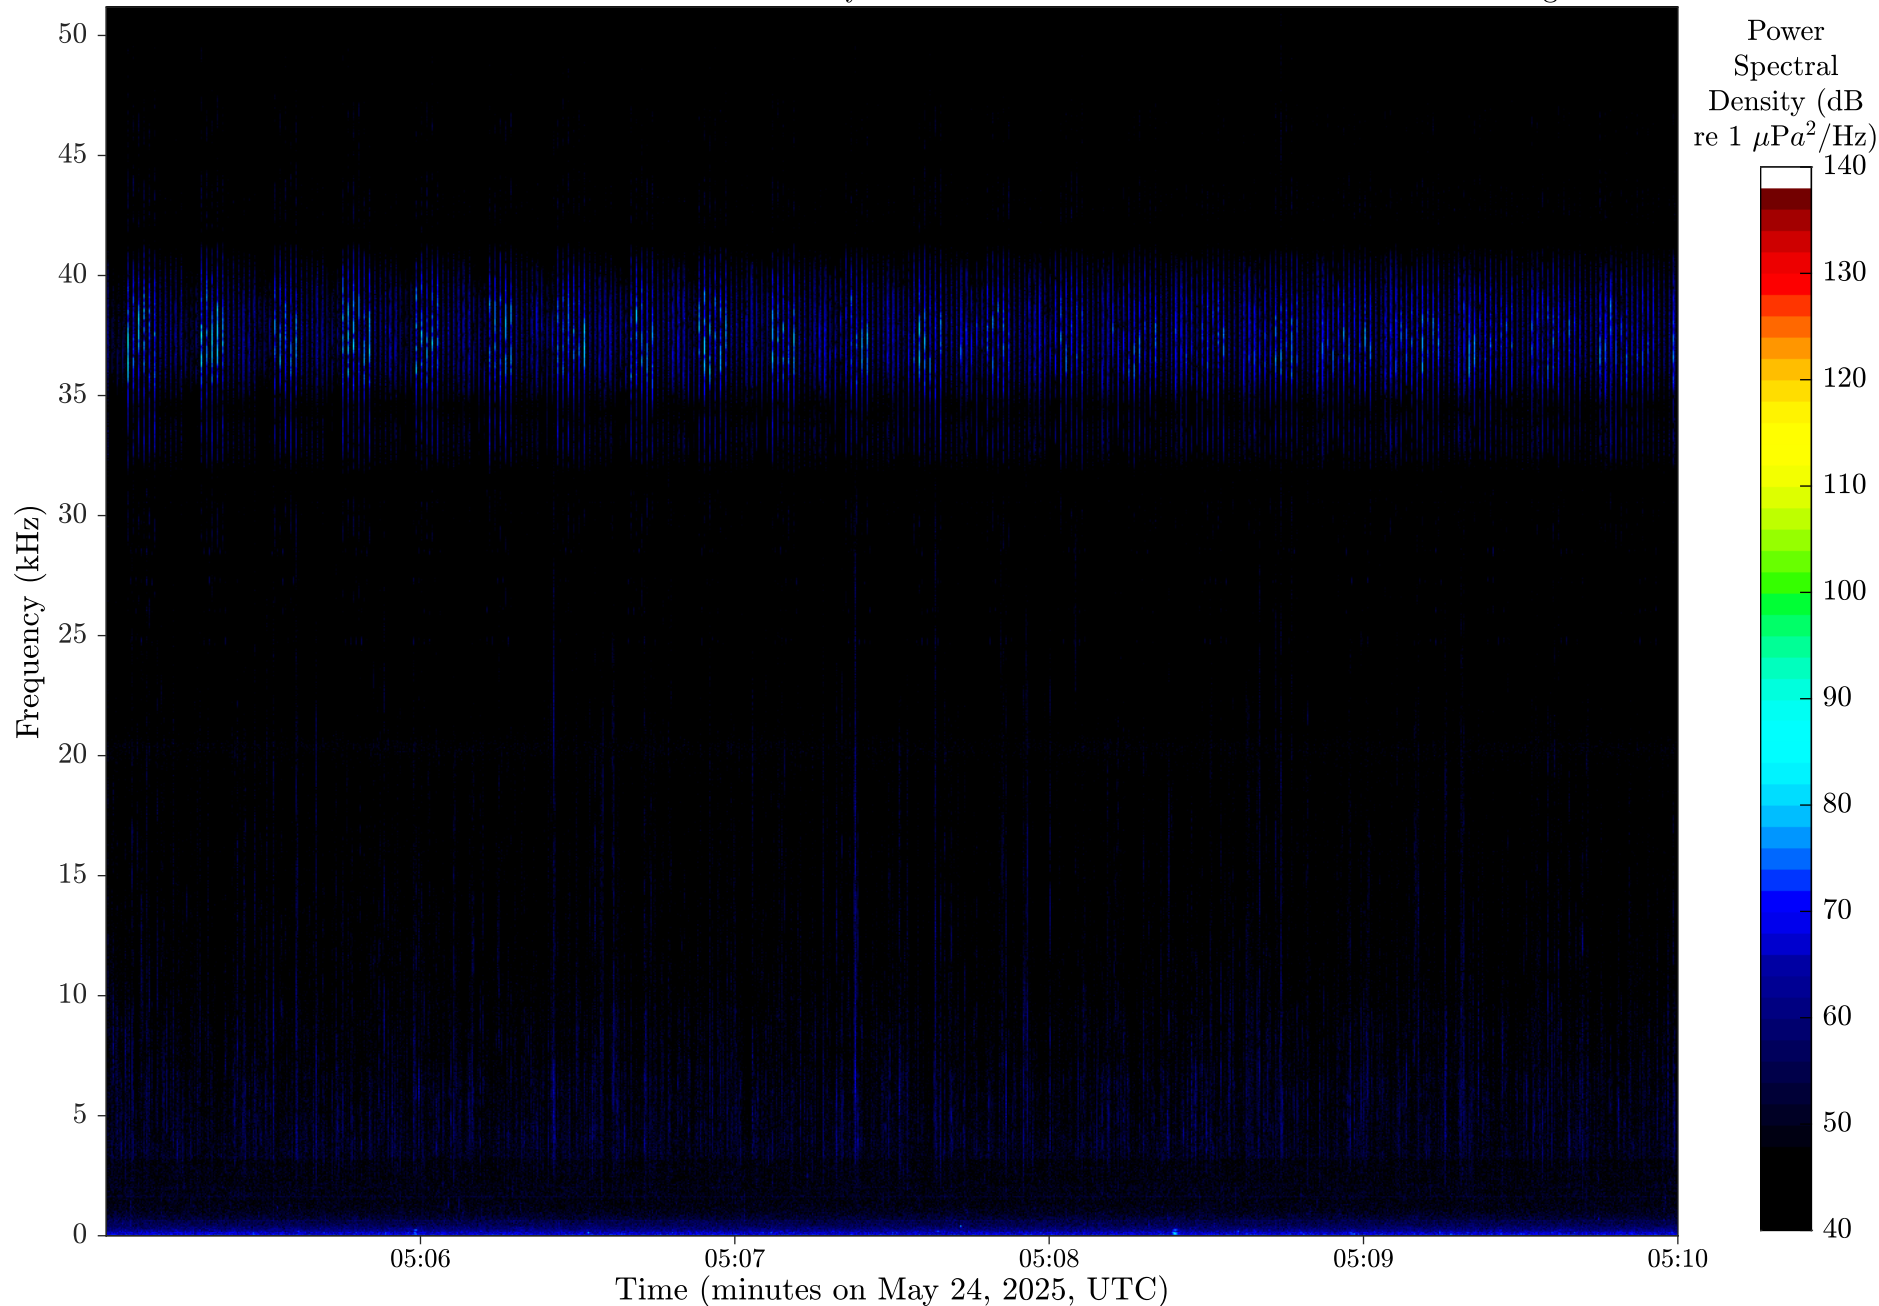


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:27:33 UTC

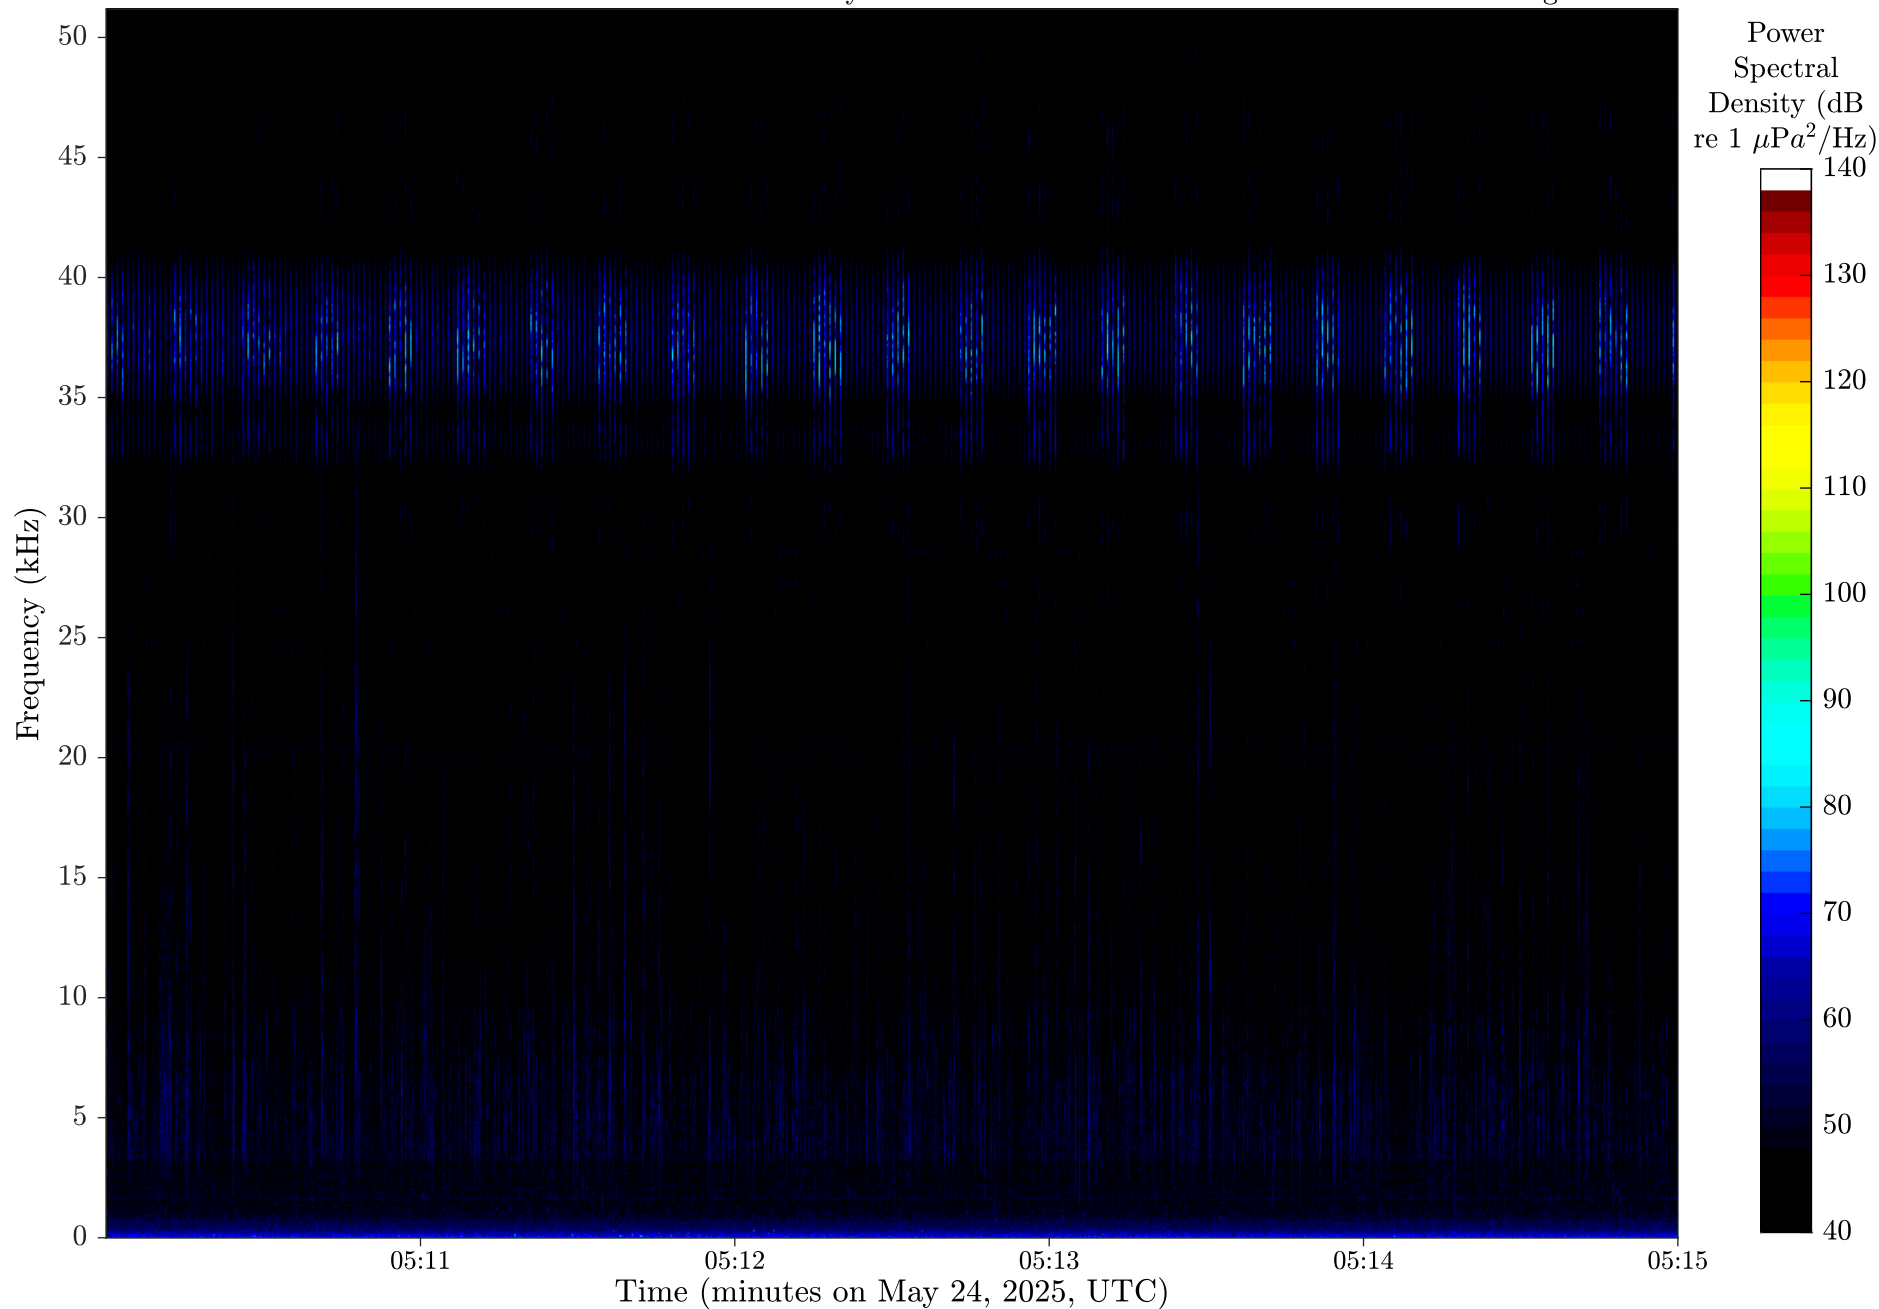

Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:27:43 UTC

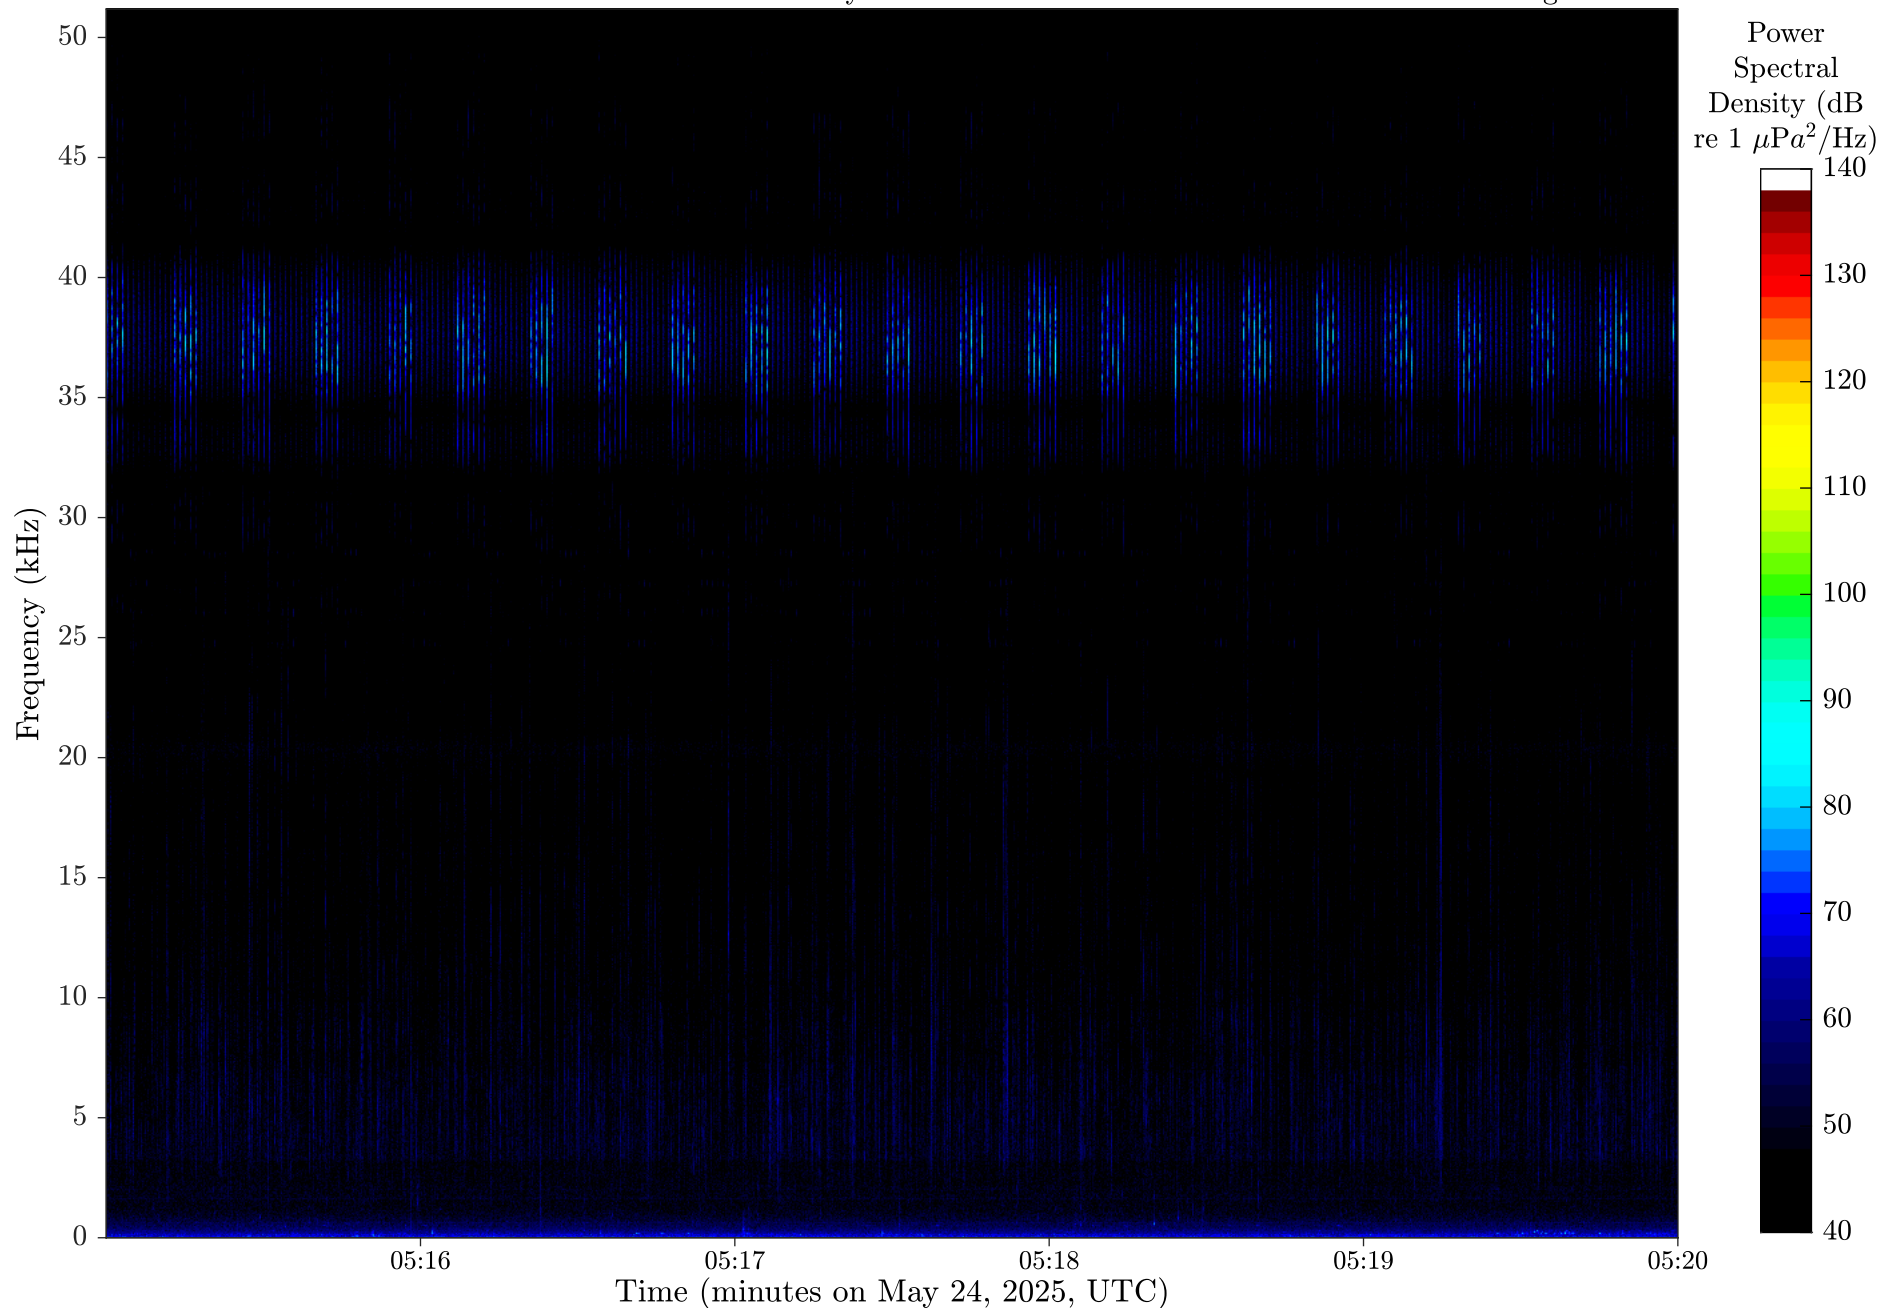

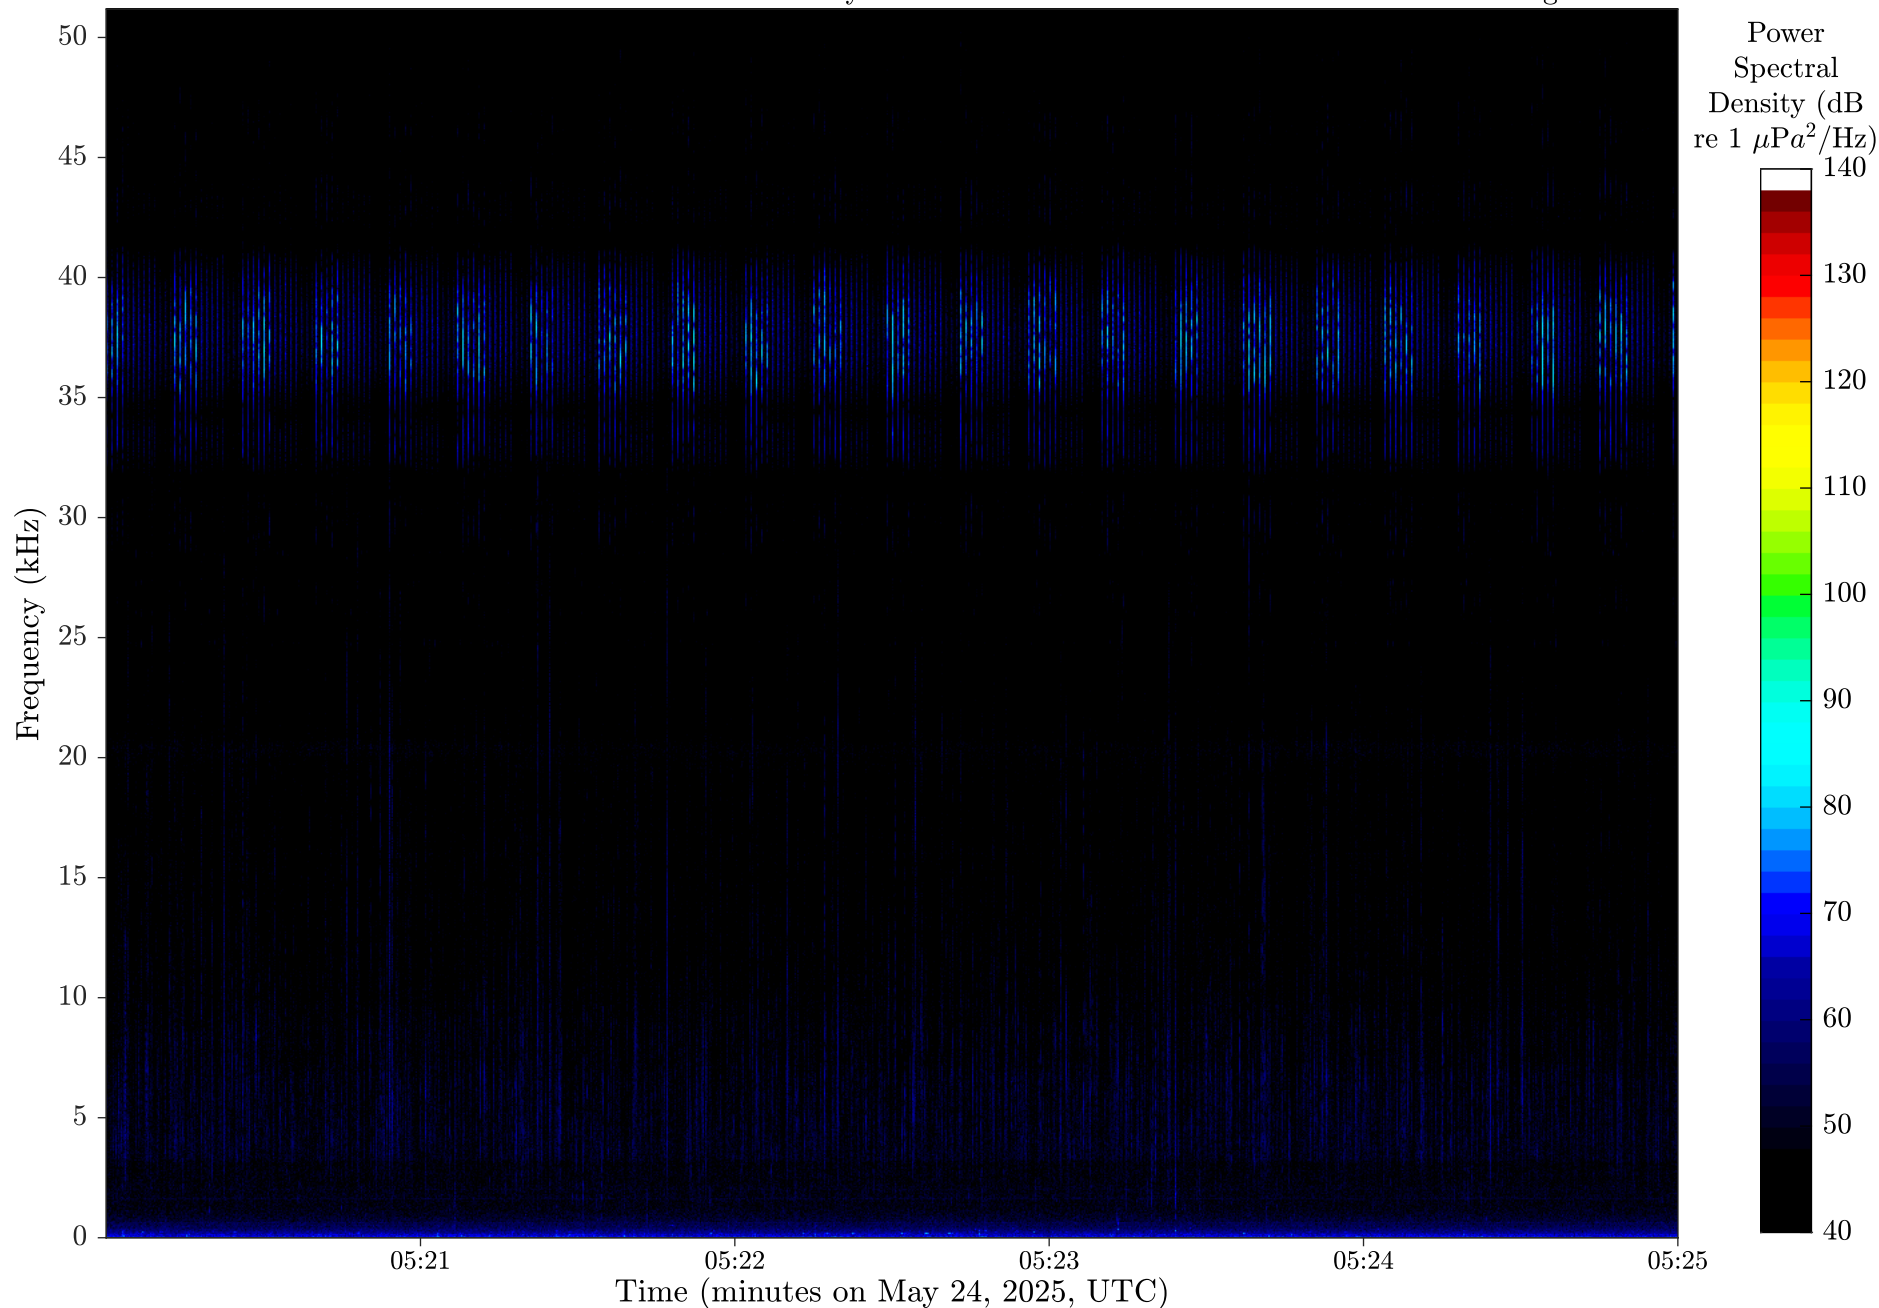


Comments: 36.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:28:00 UTC

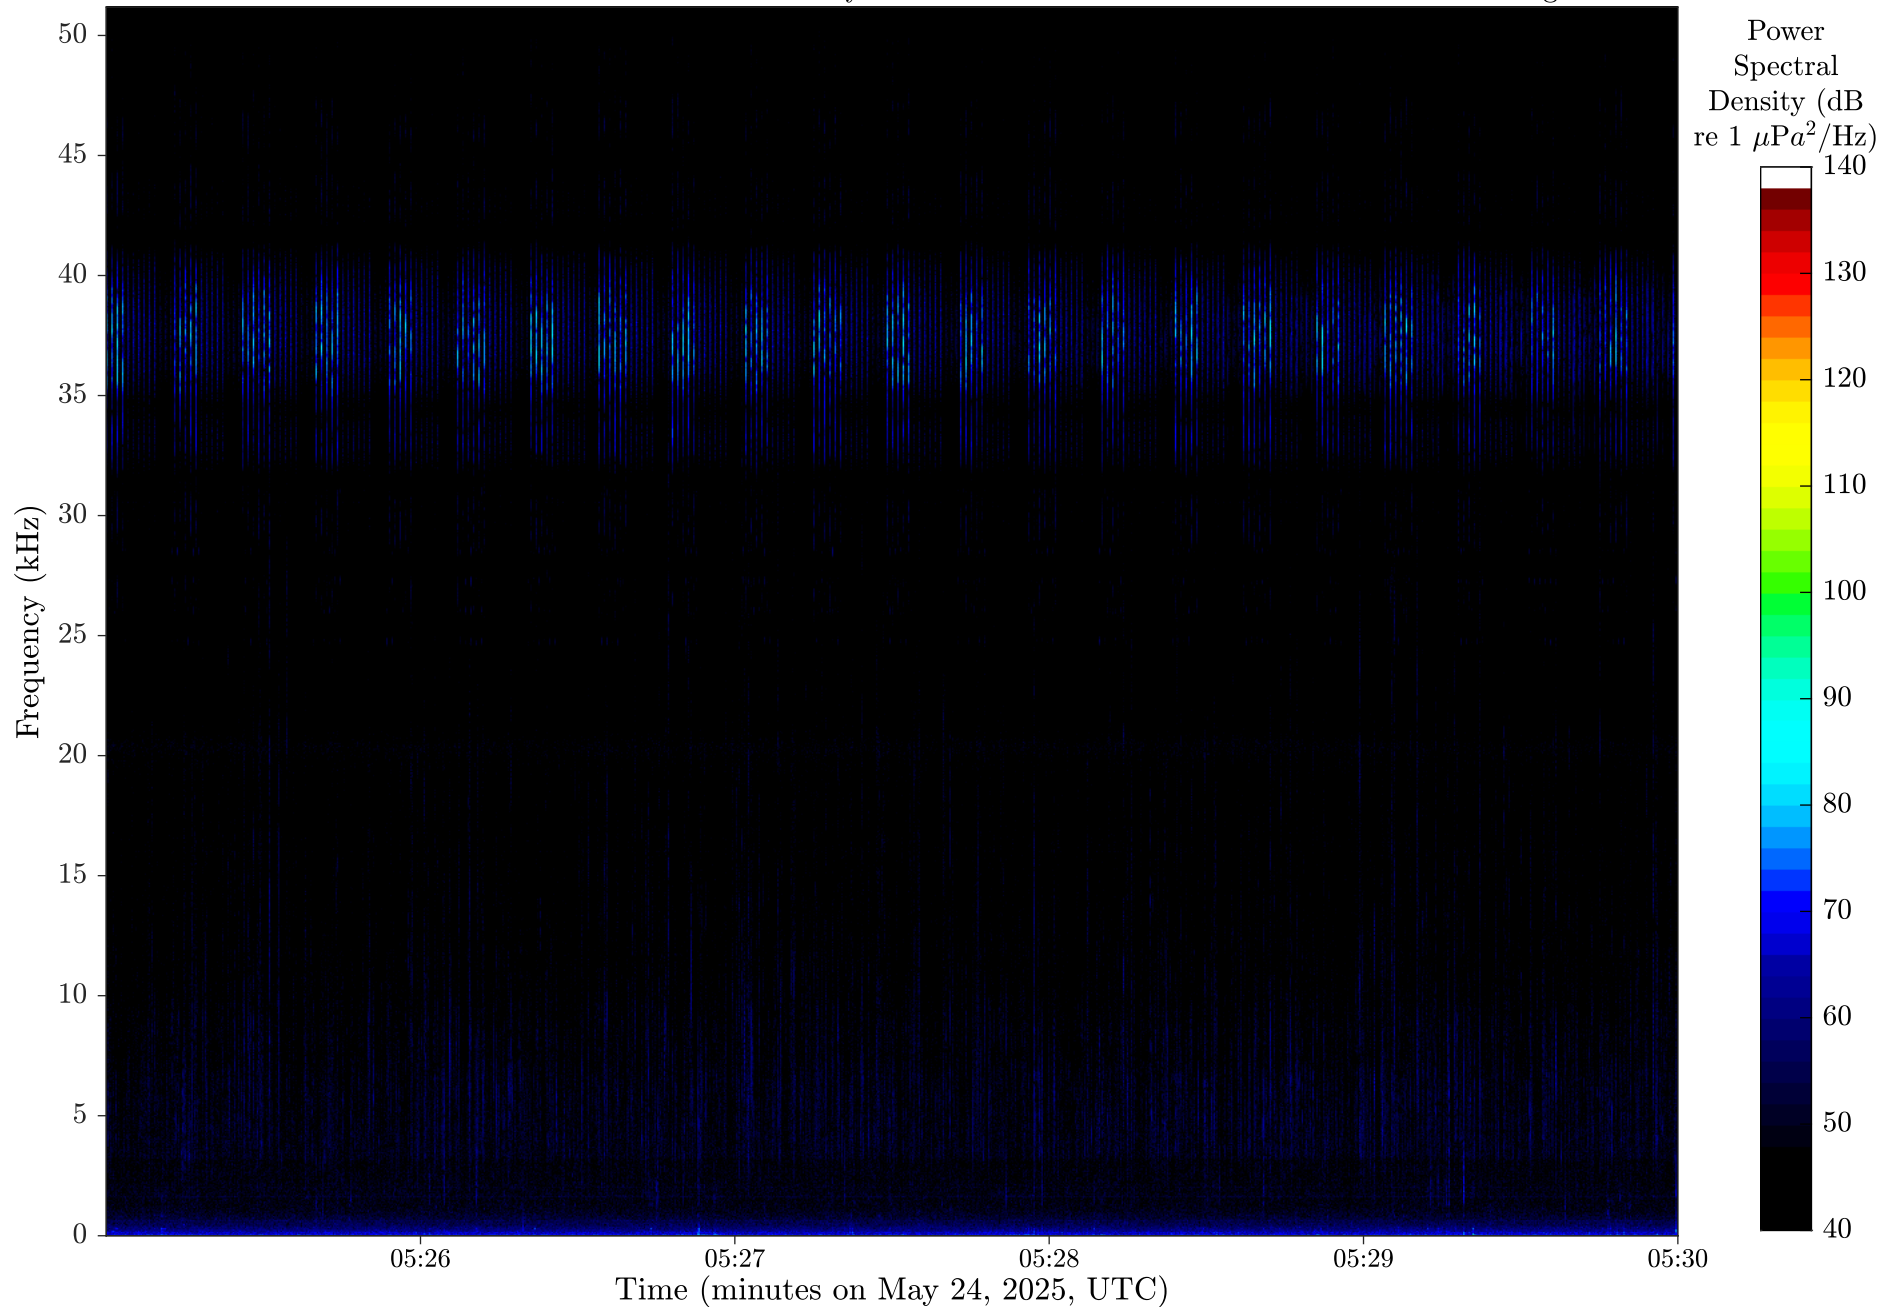


Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:28:08 UTC

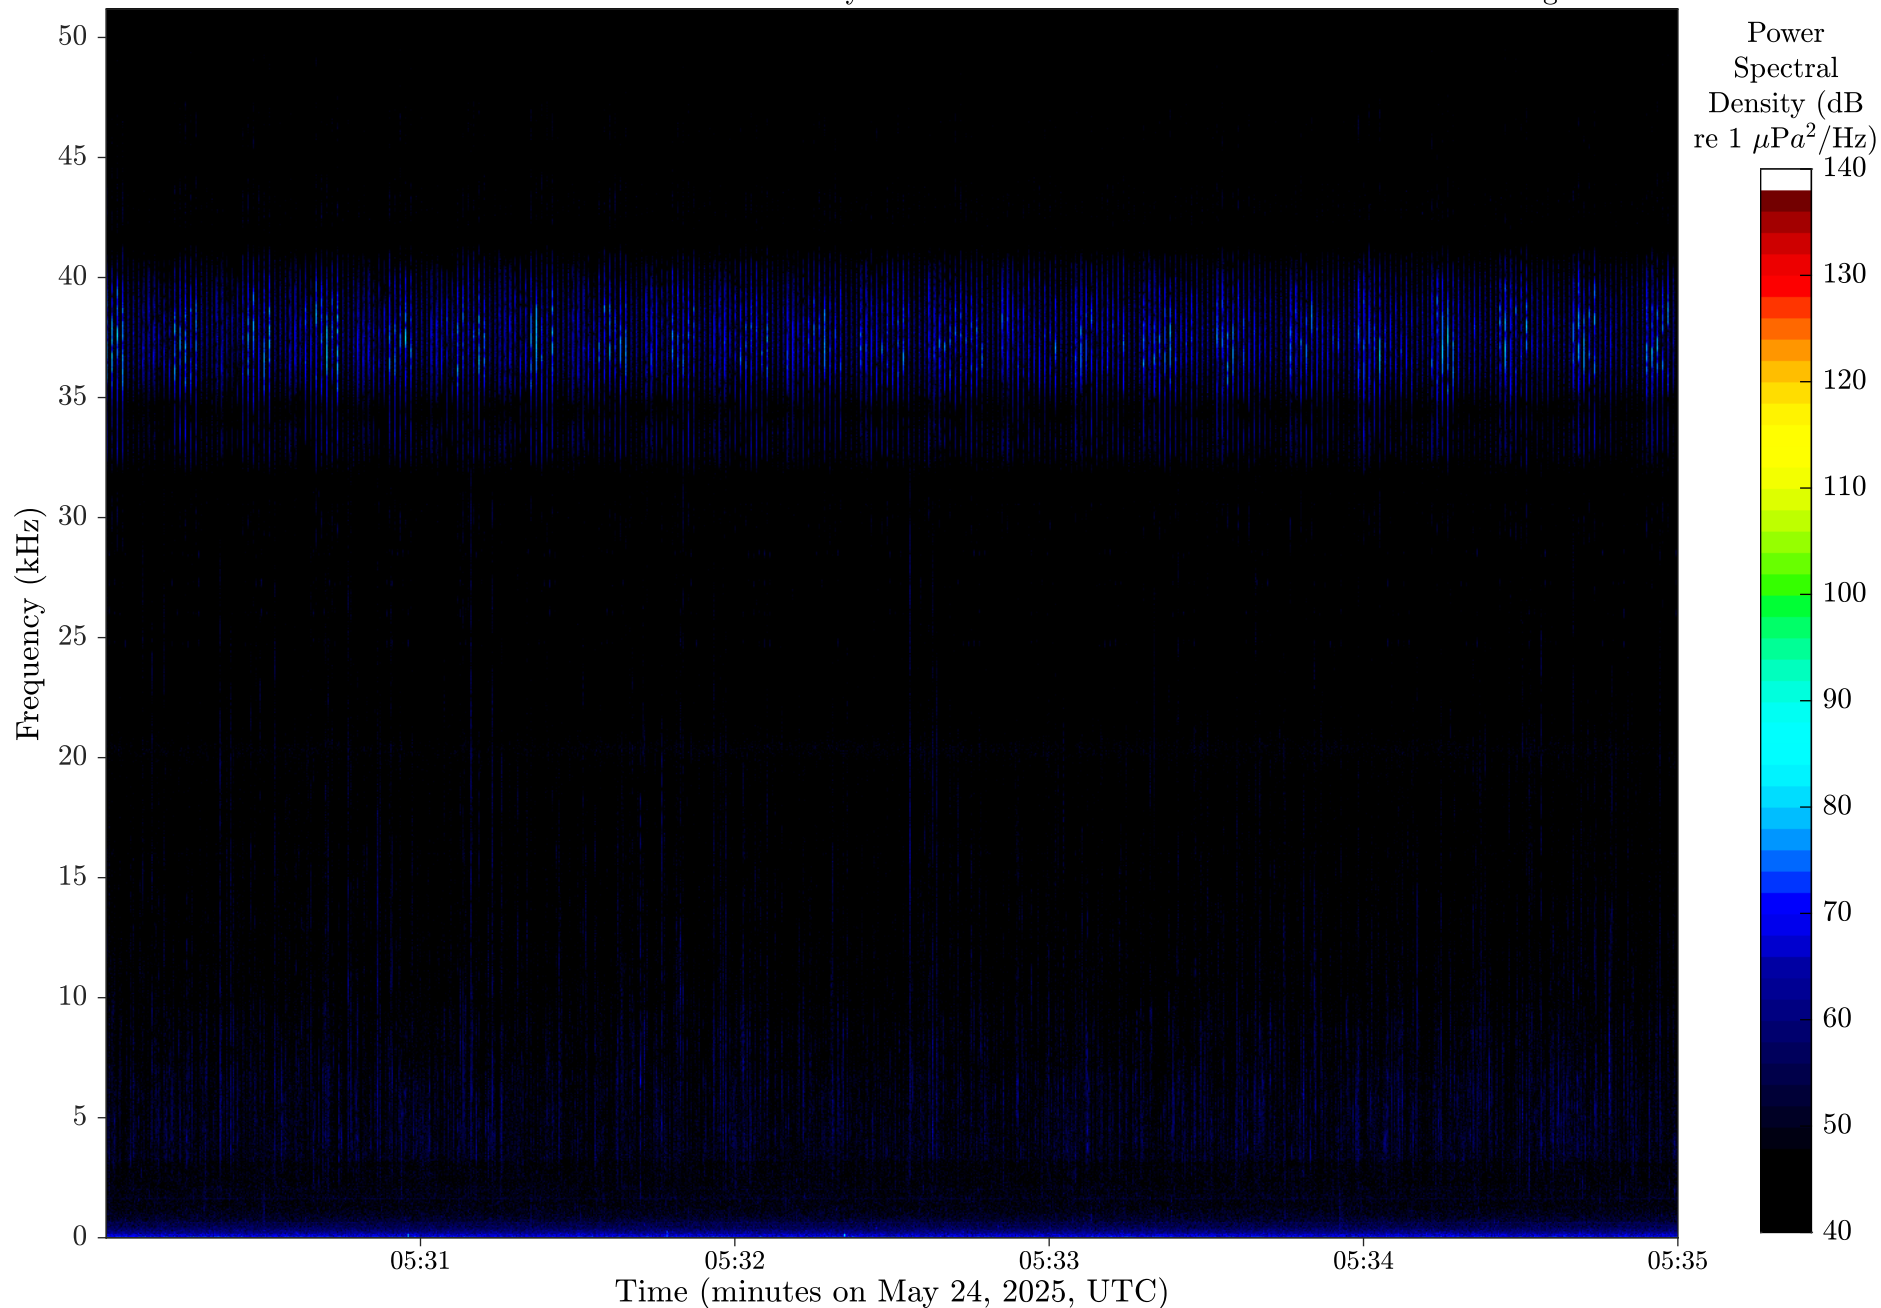


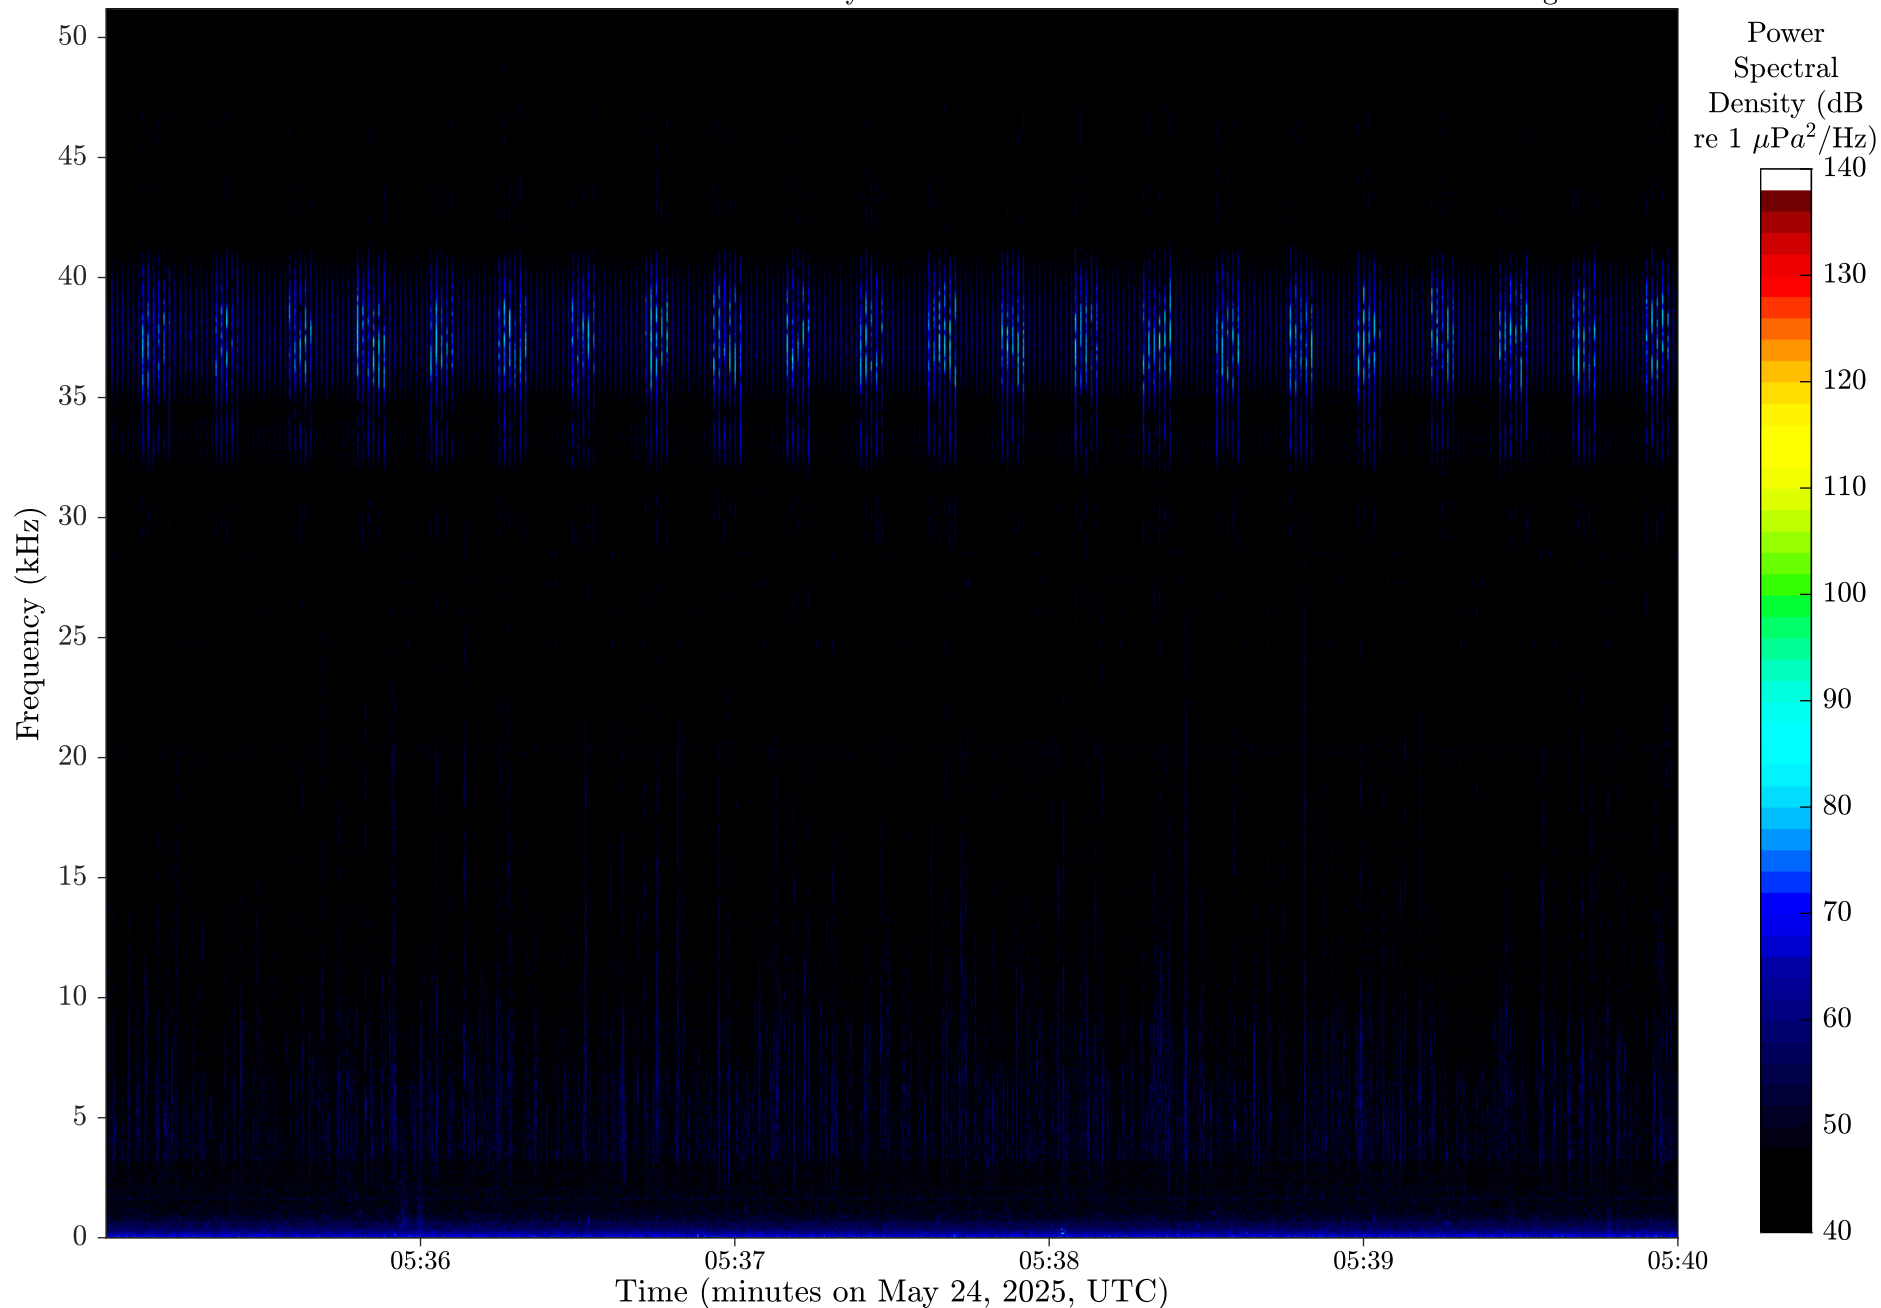

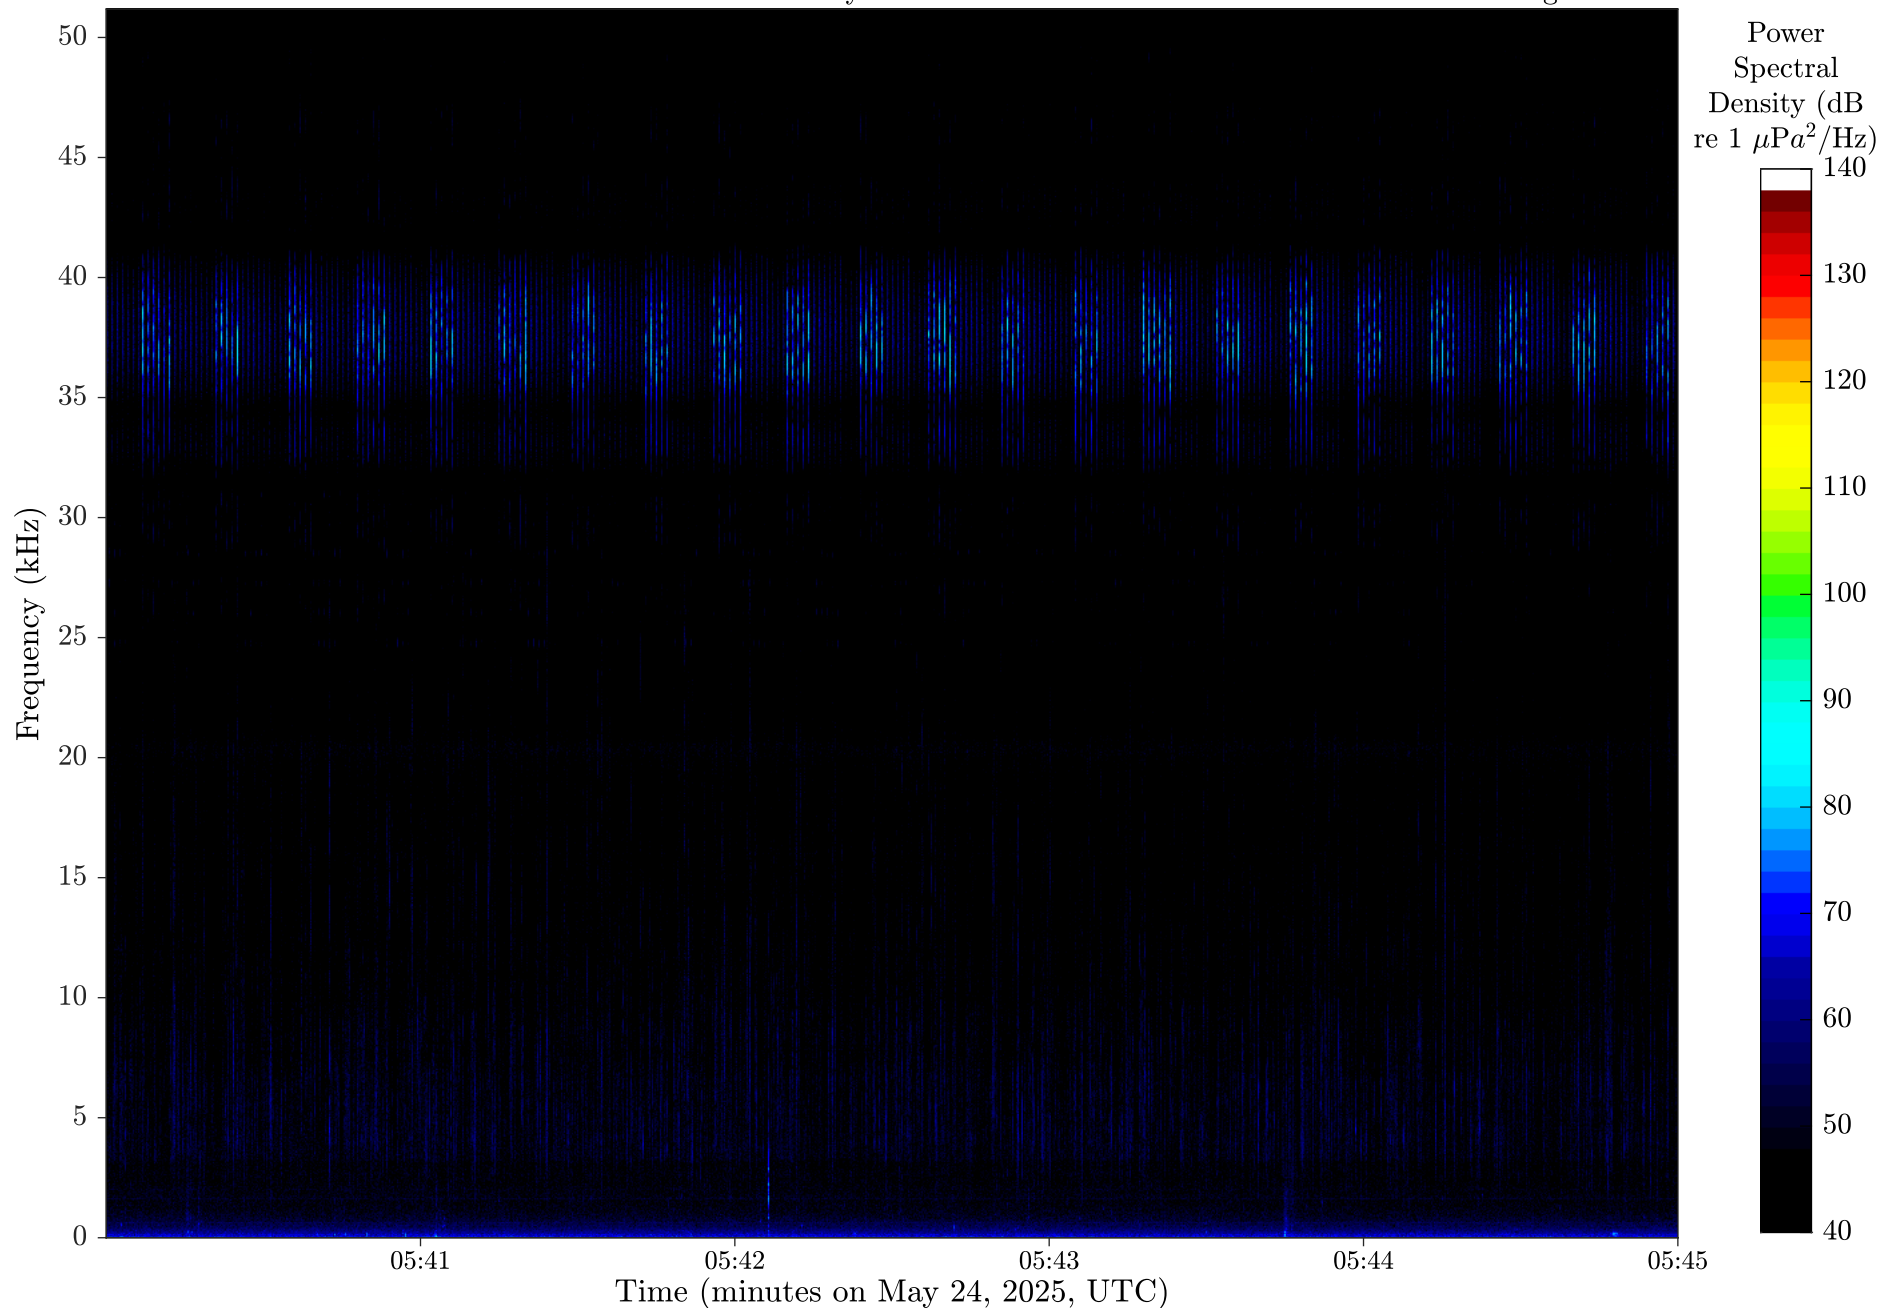


Comments: 36.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:28:33 UTC

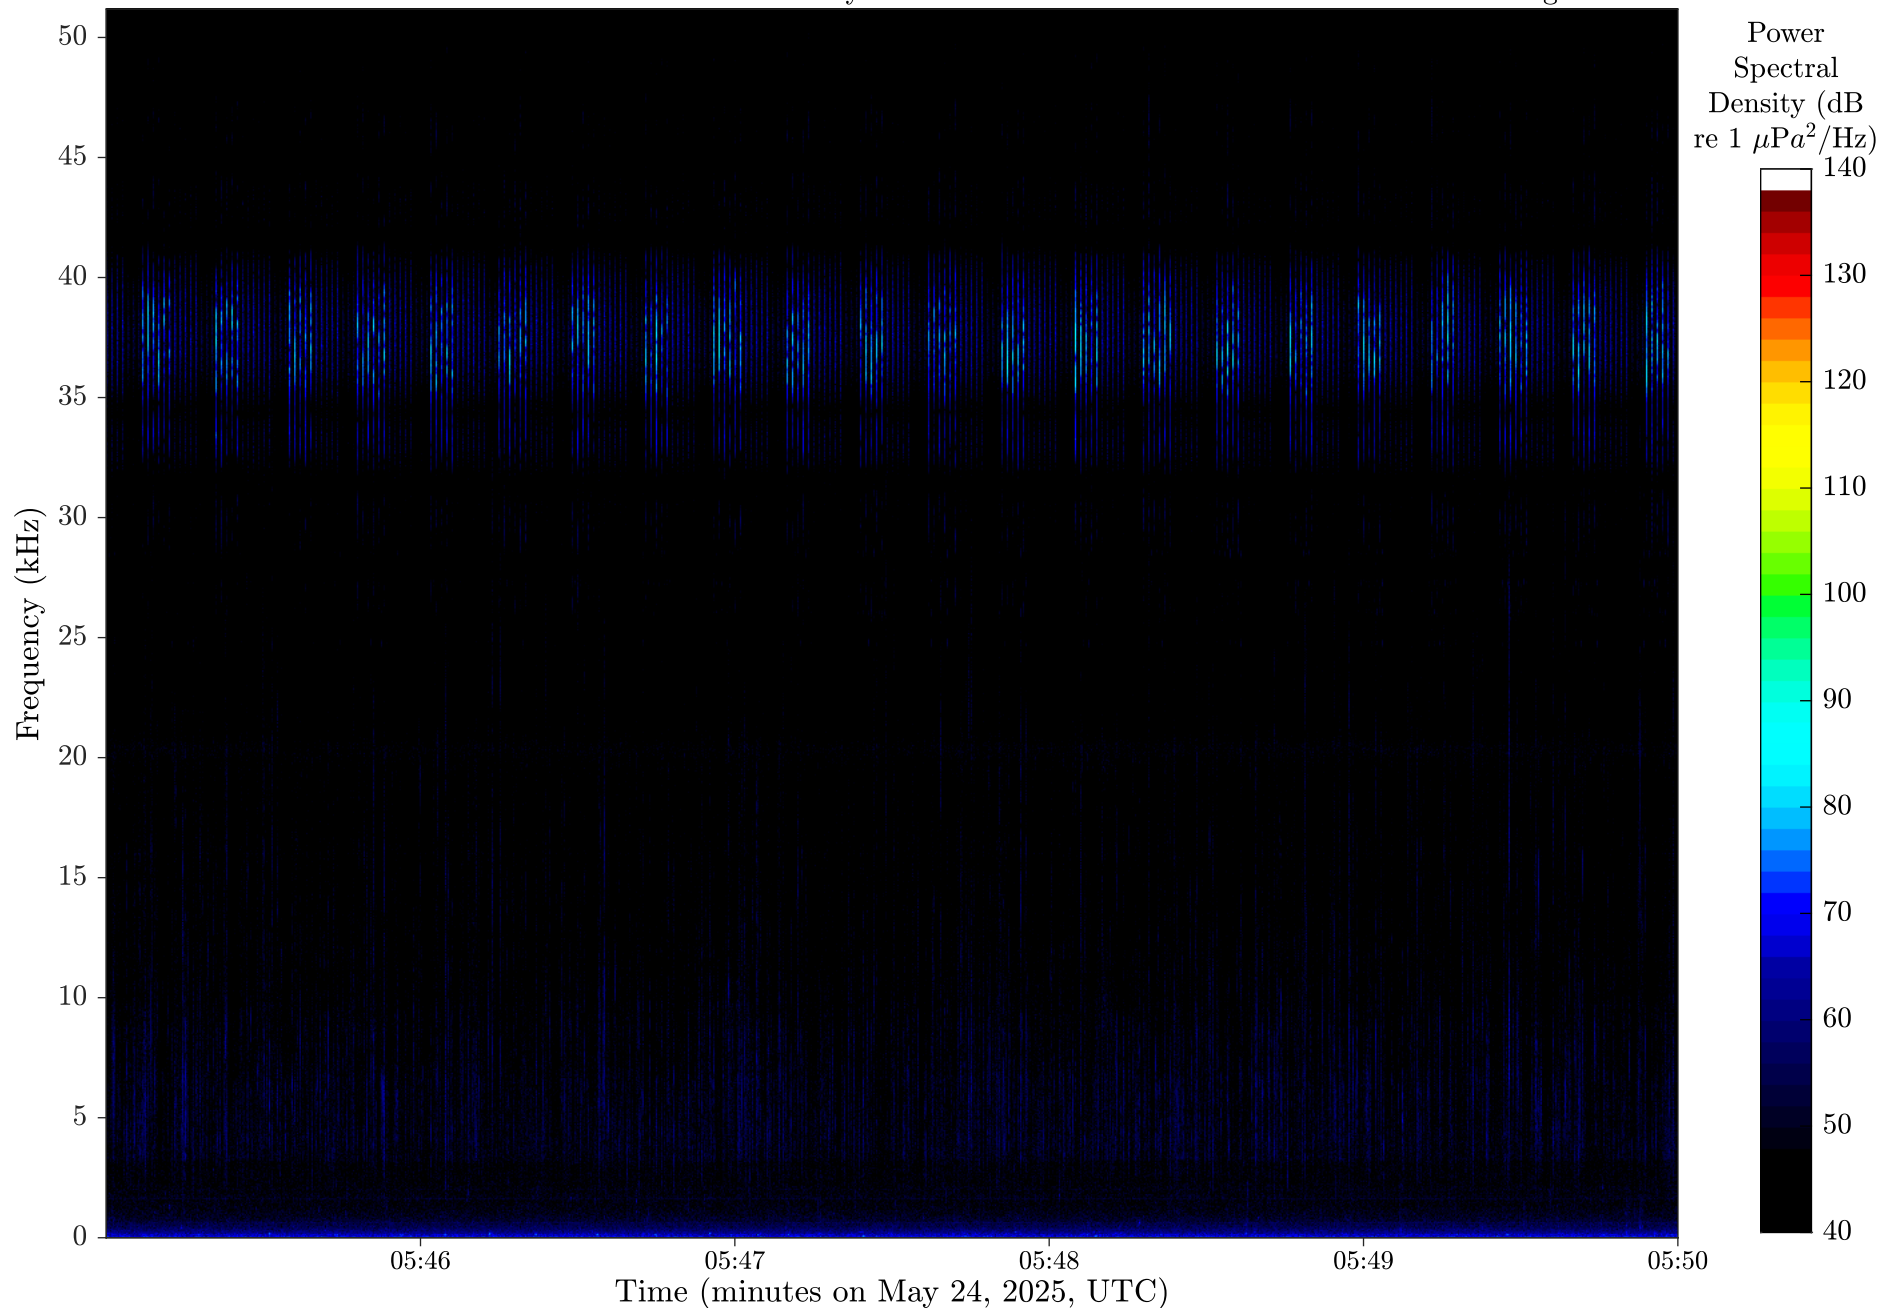



Comments: 36.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:28:41 UTC

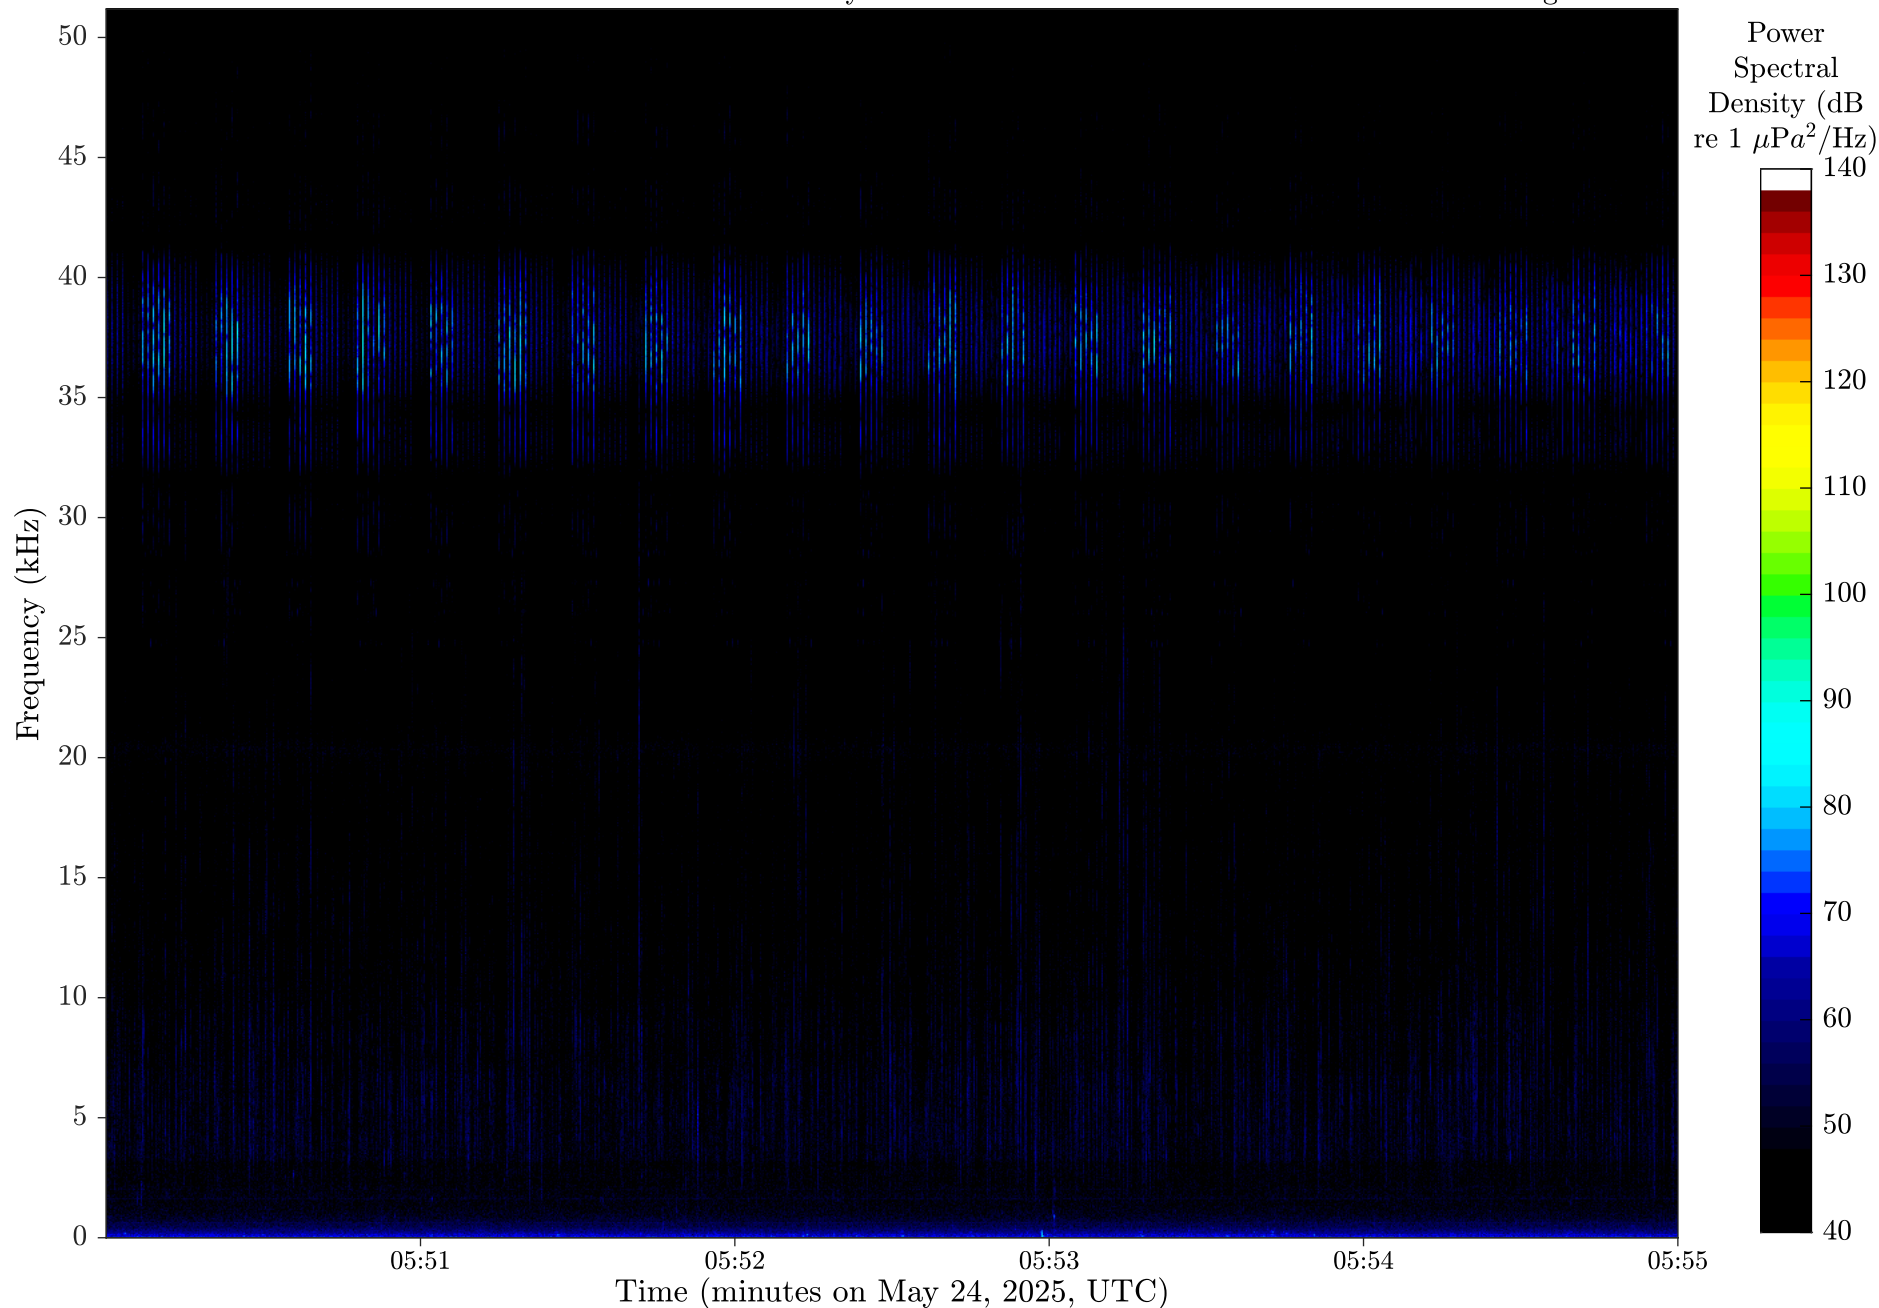

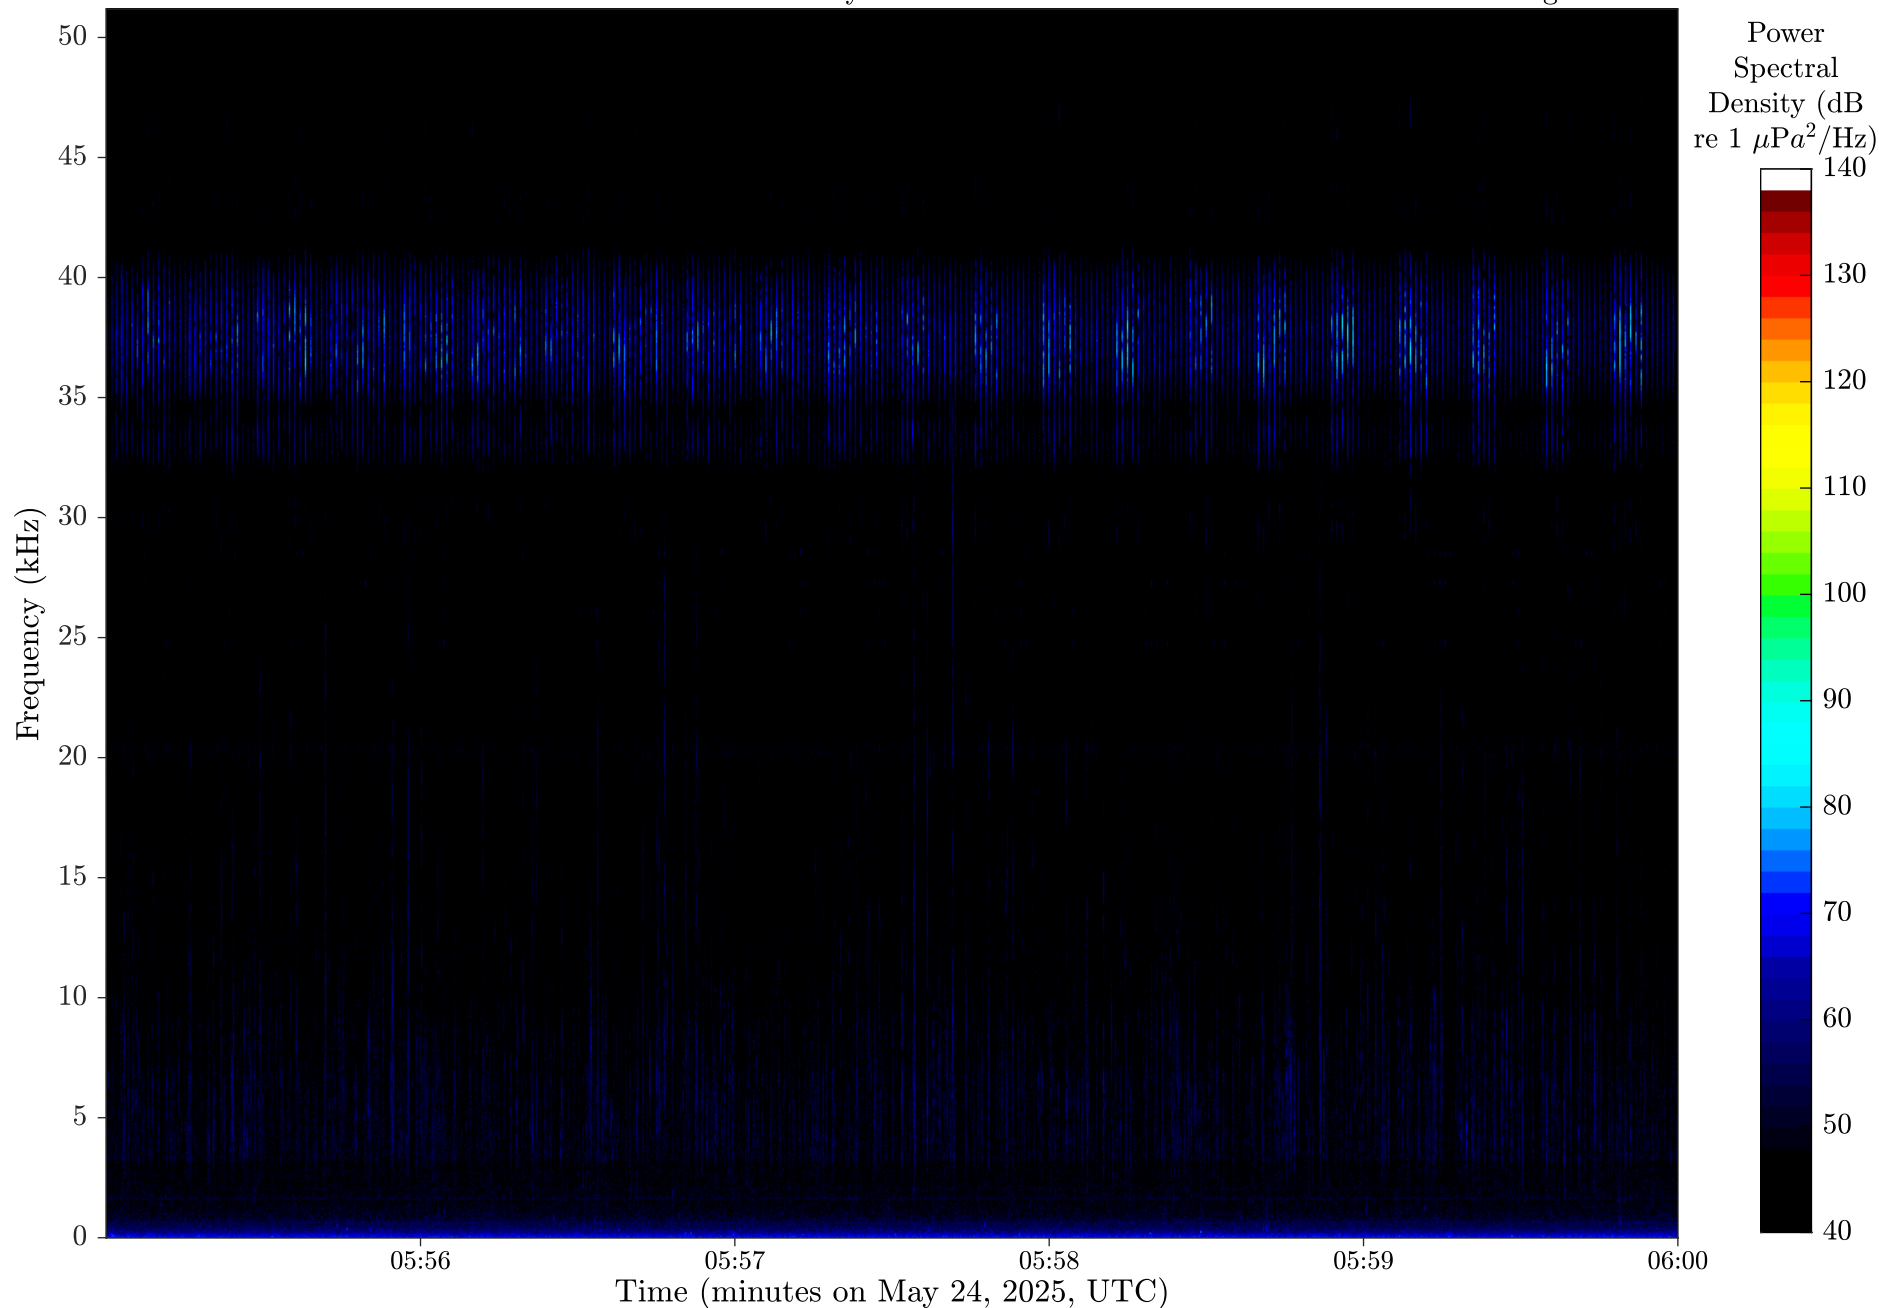


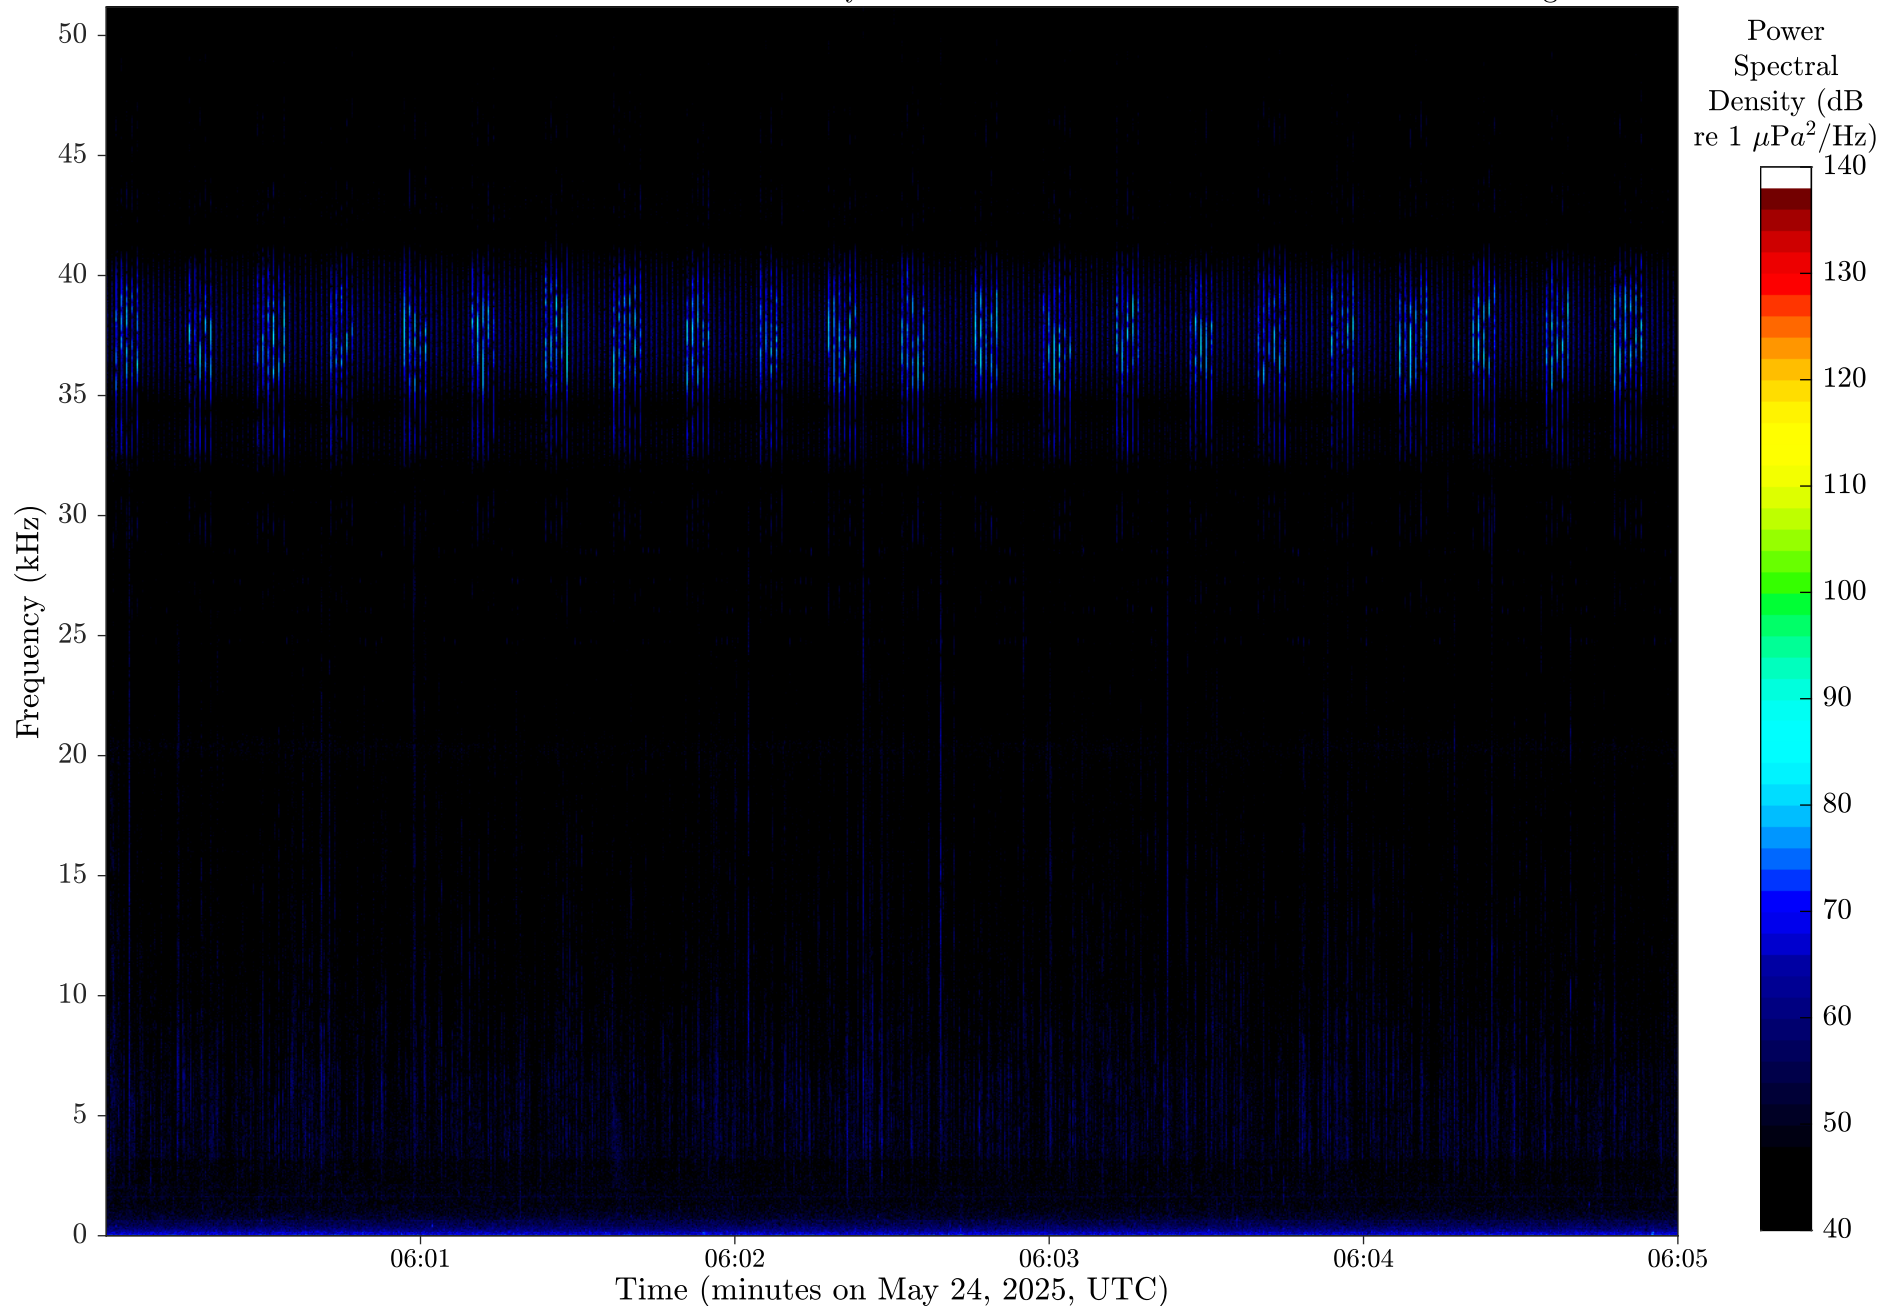

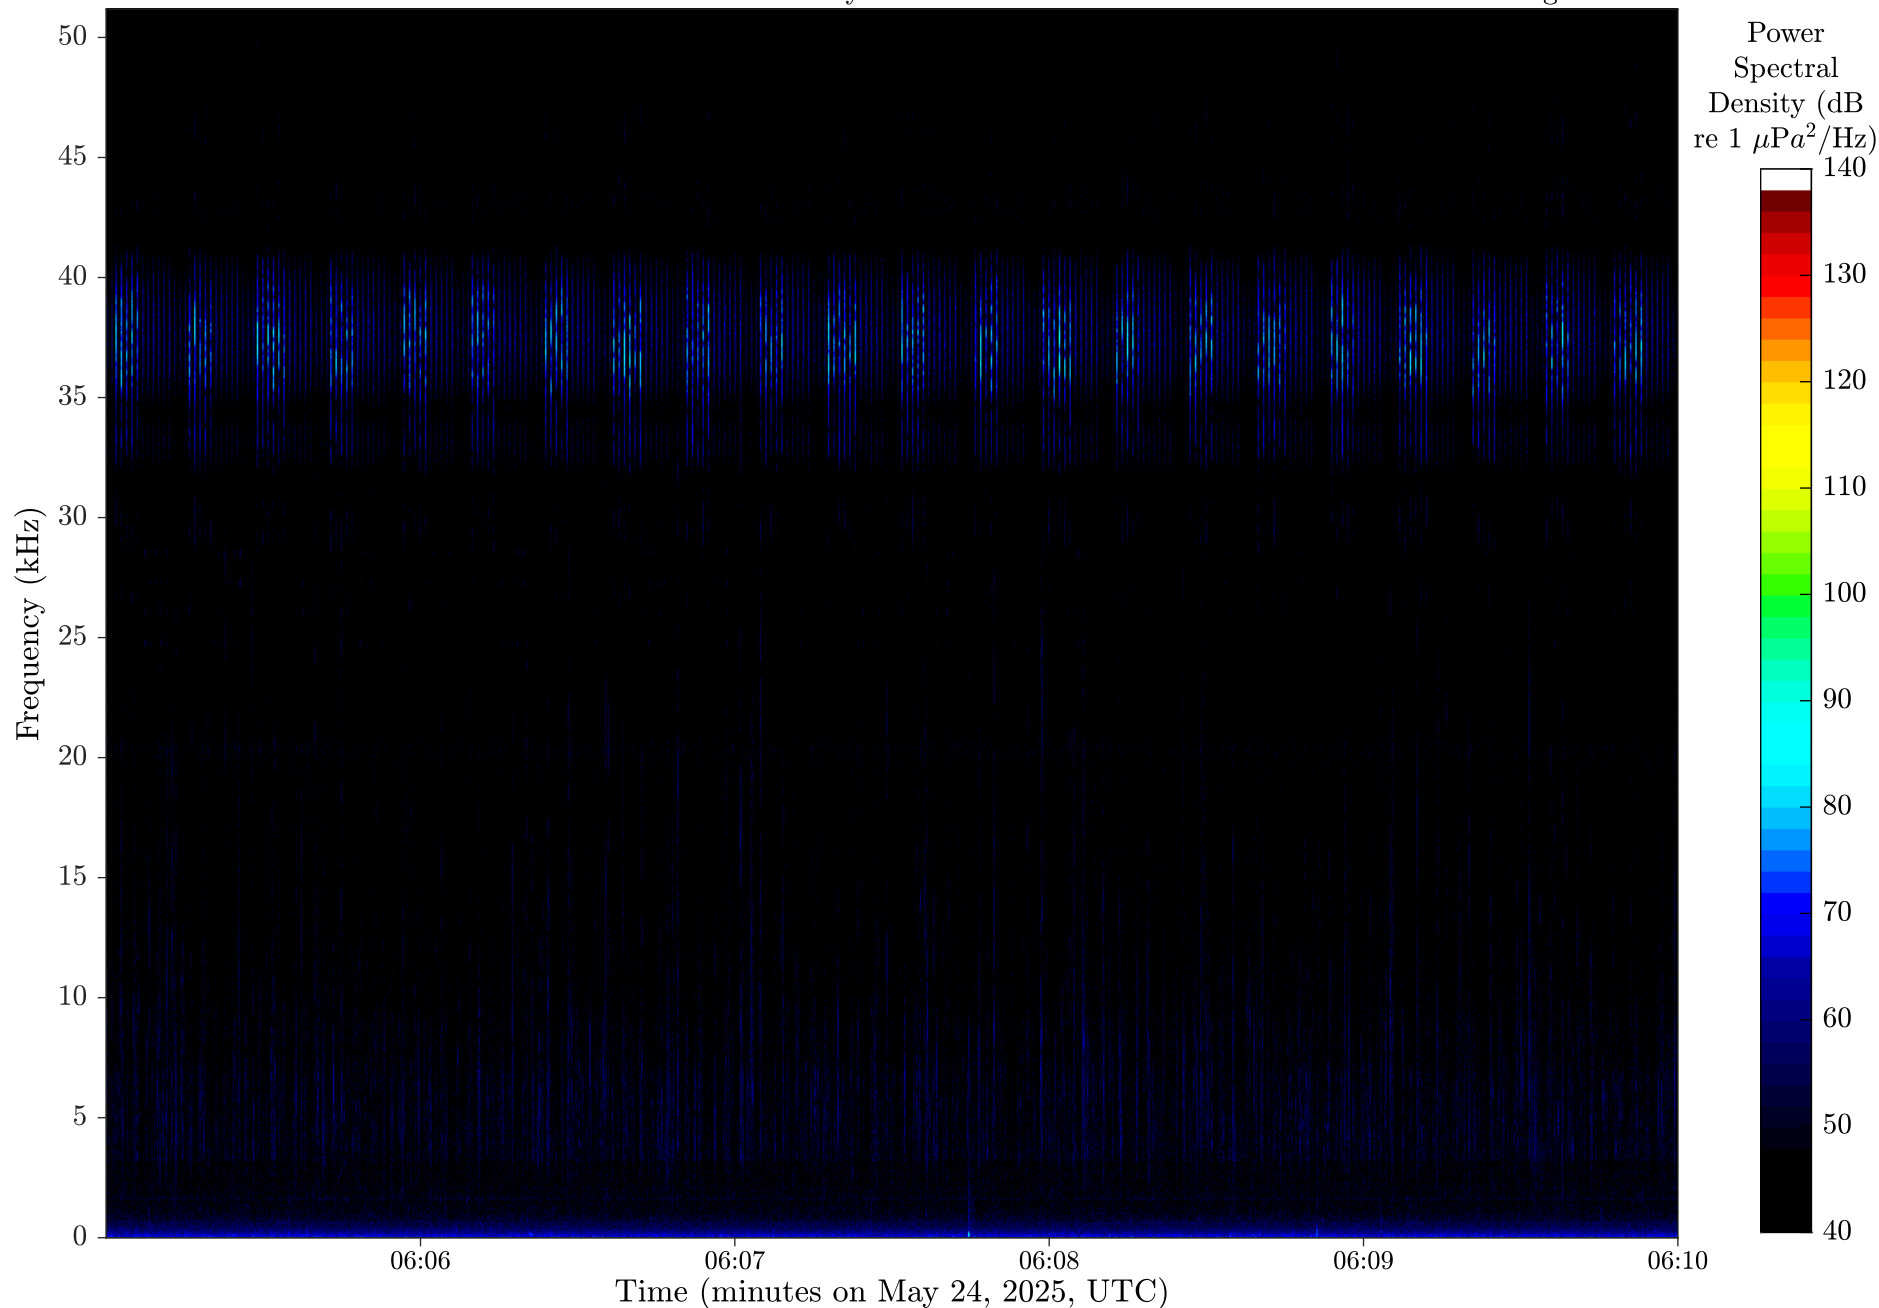


Comments: 36.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:15 UTC

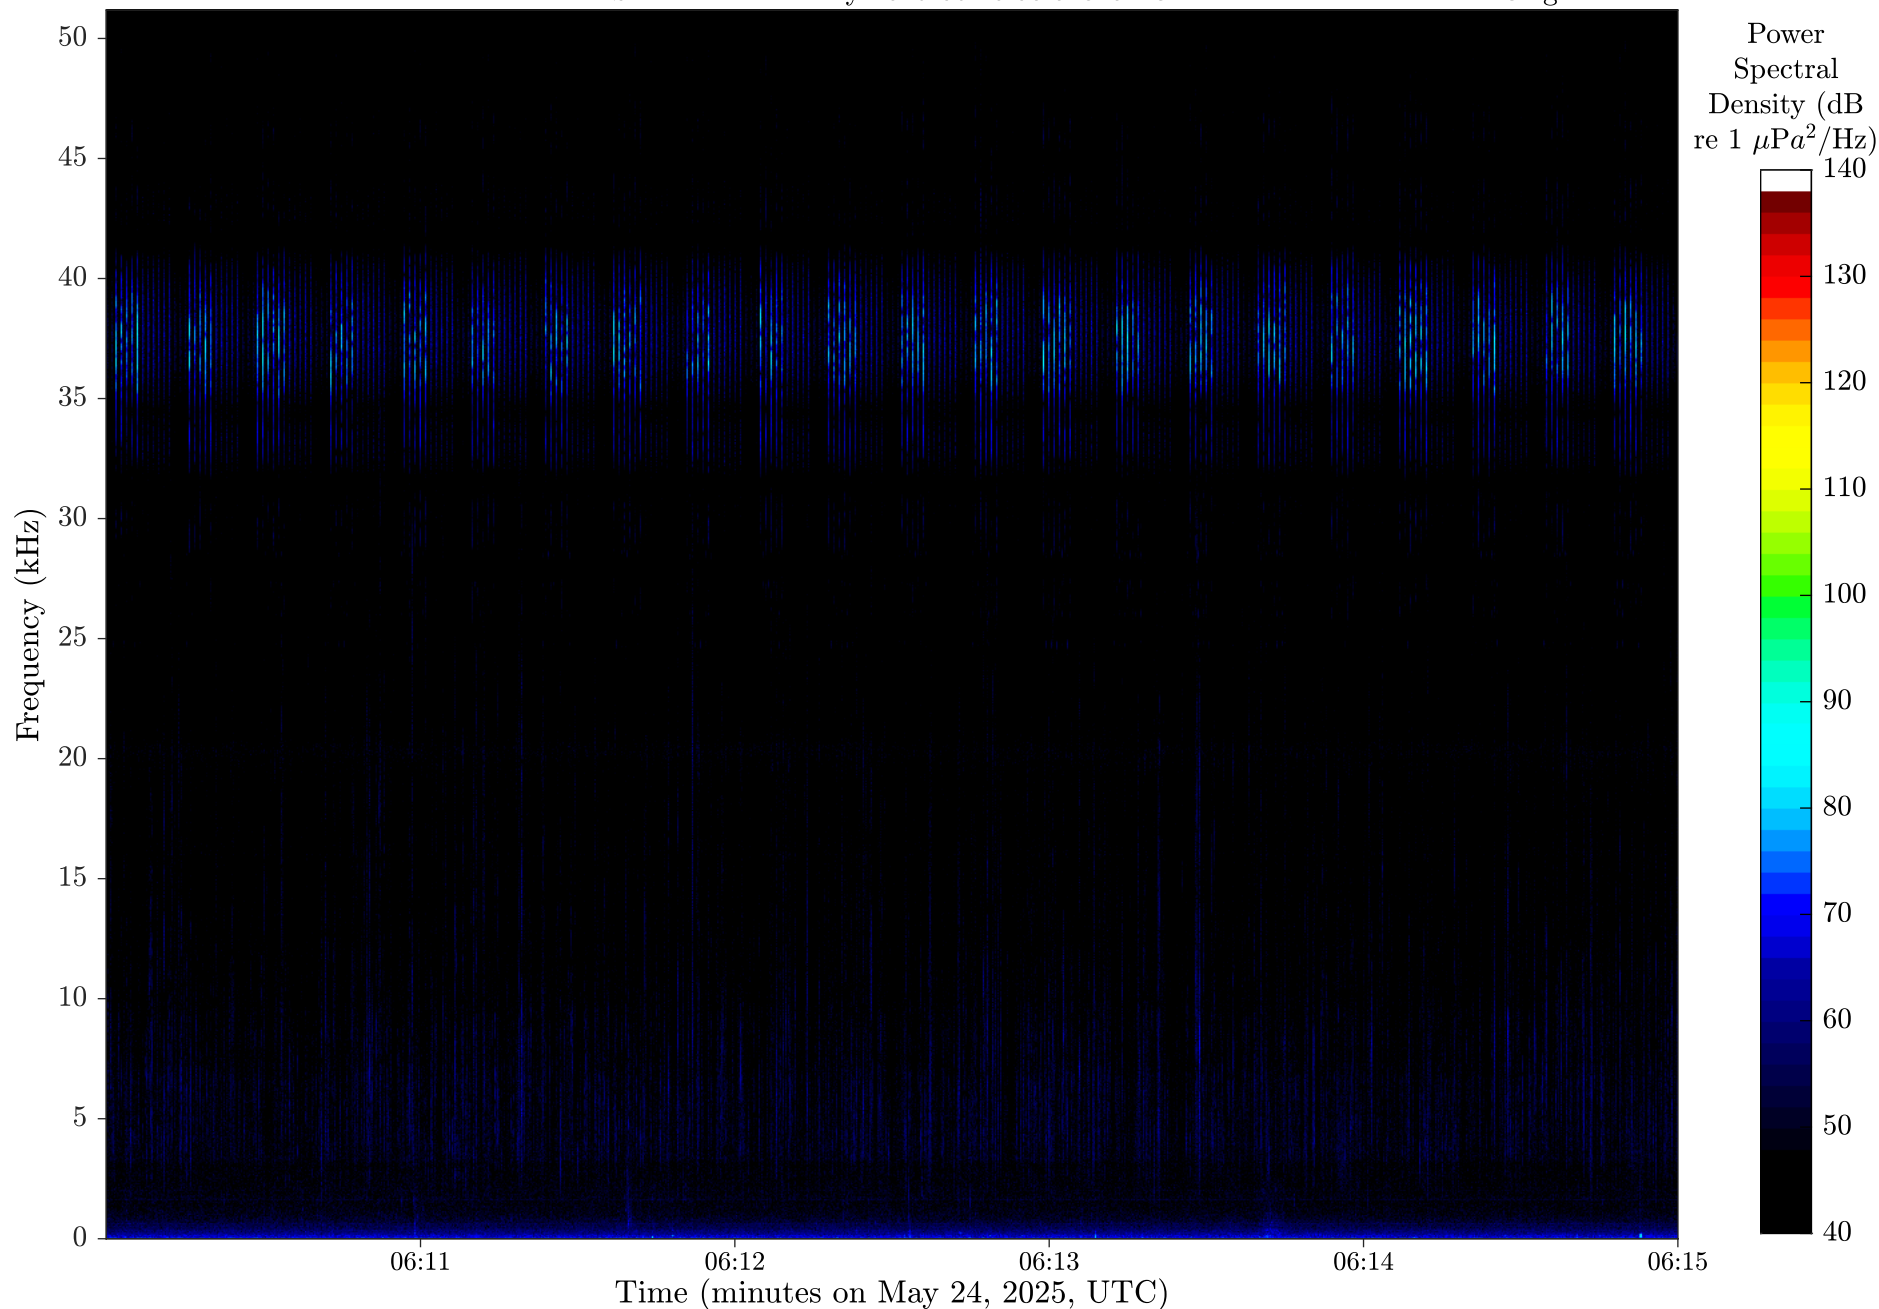


Comments: 36.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:23 UTC

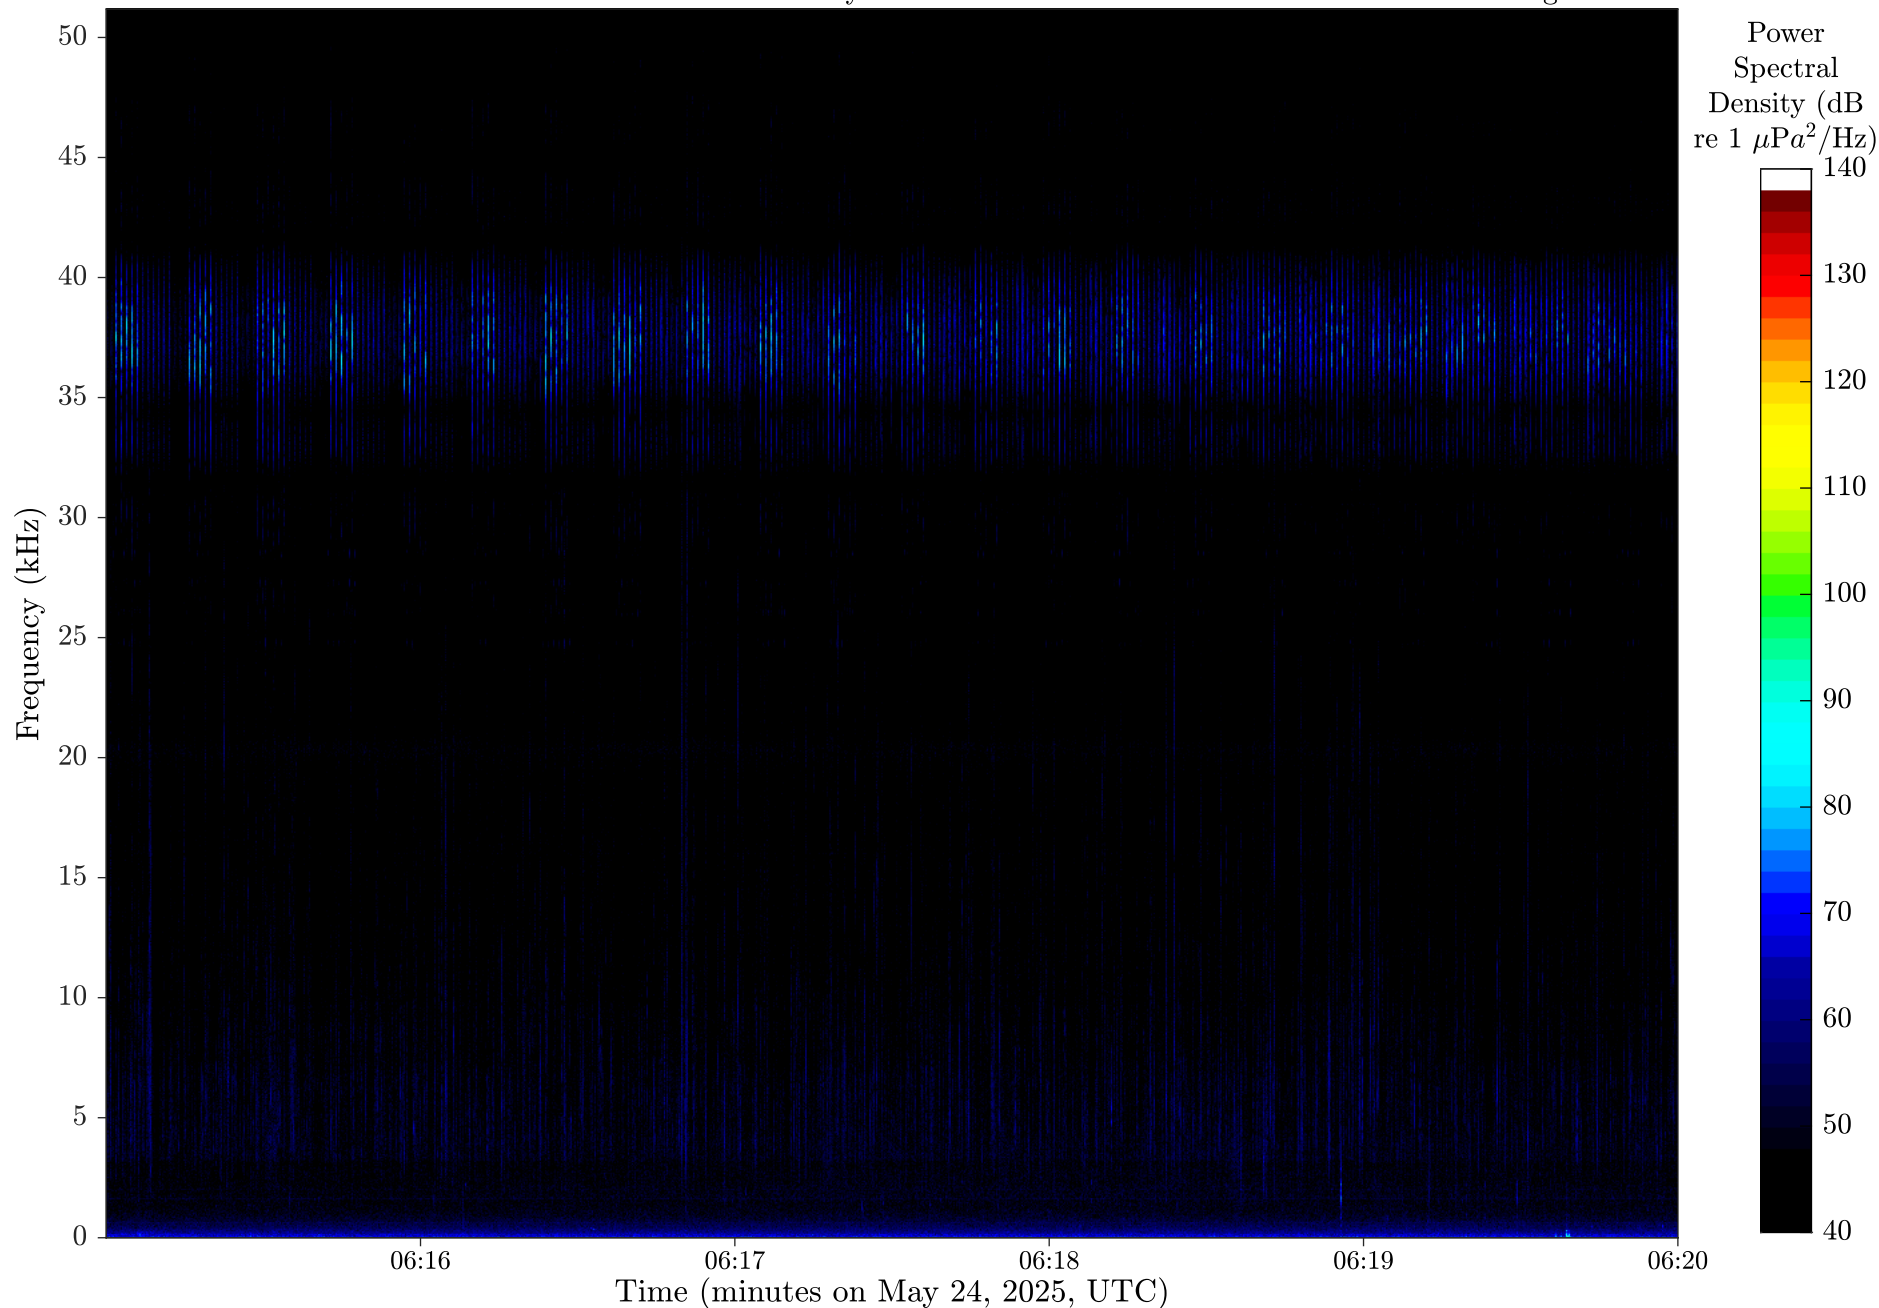


Comments: 36 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:31 UTC

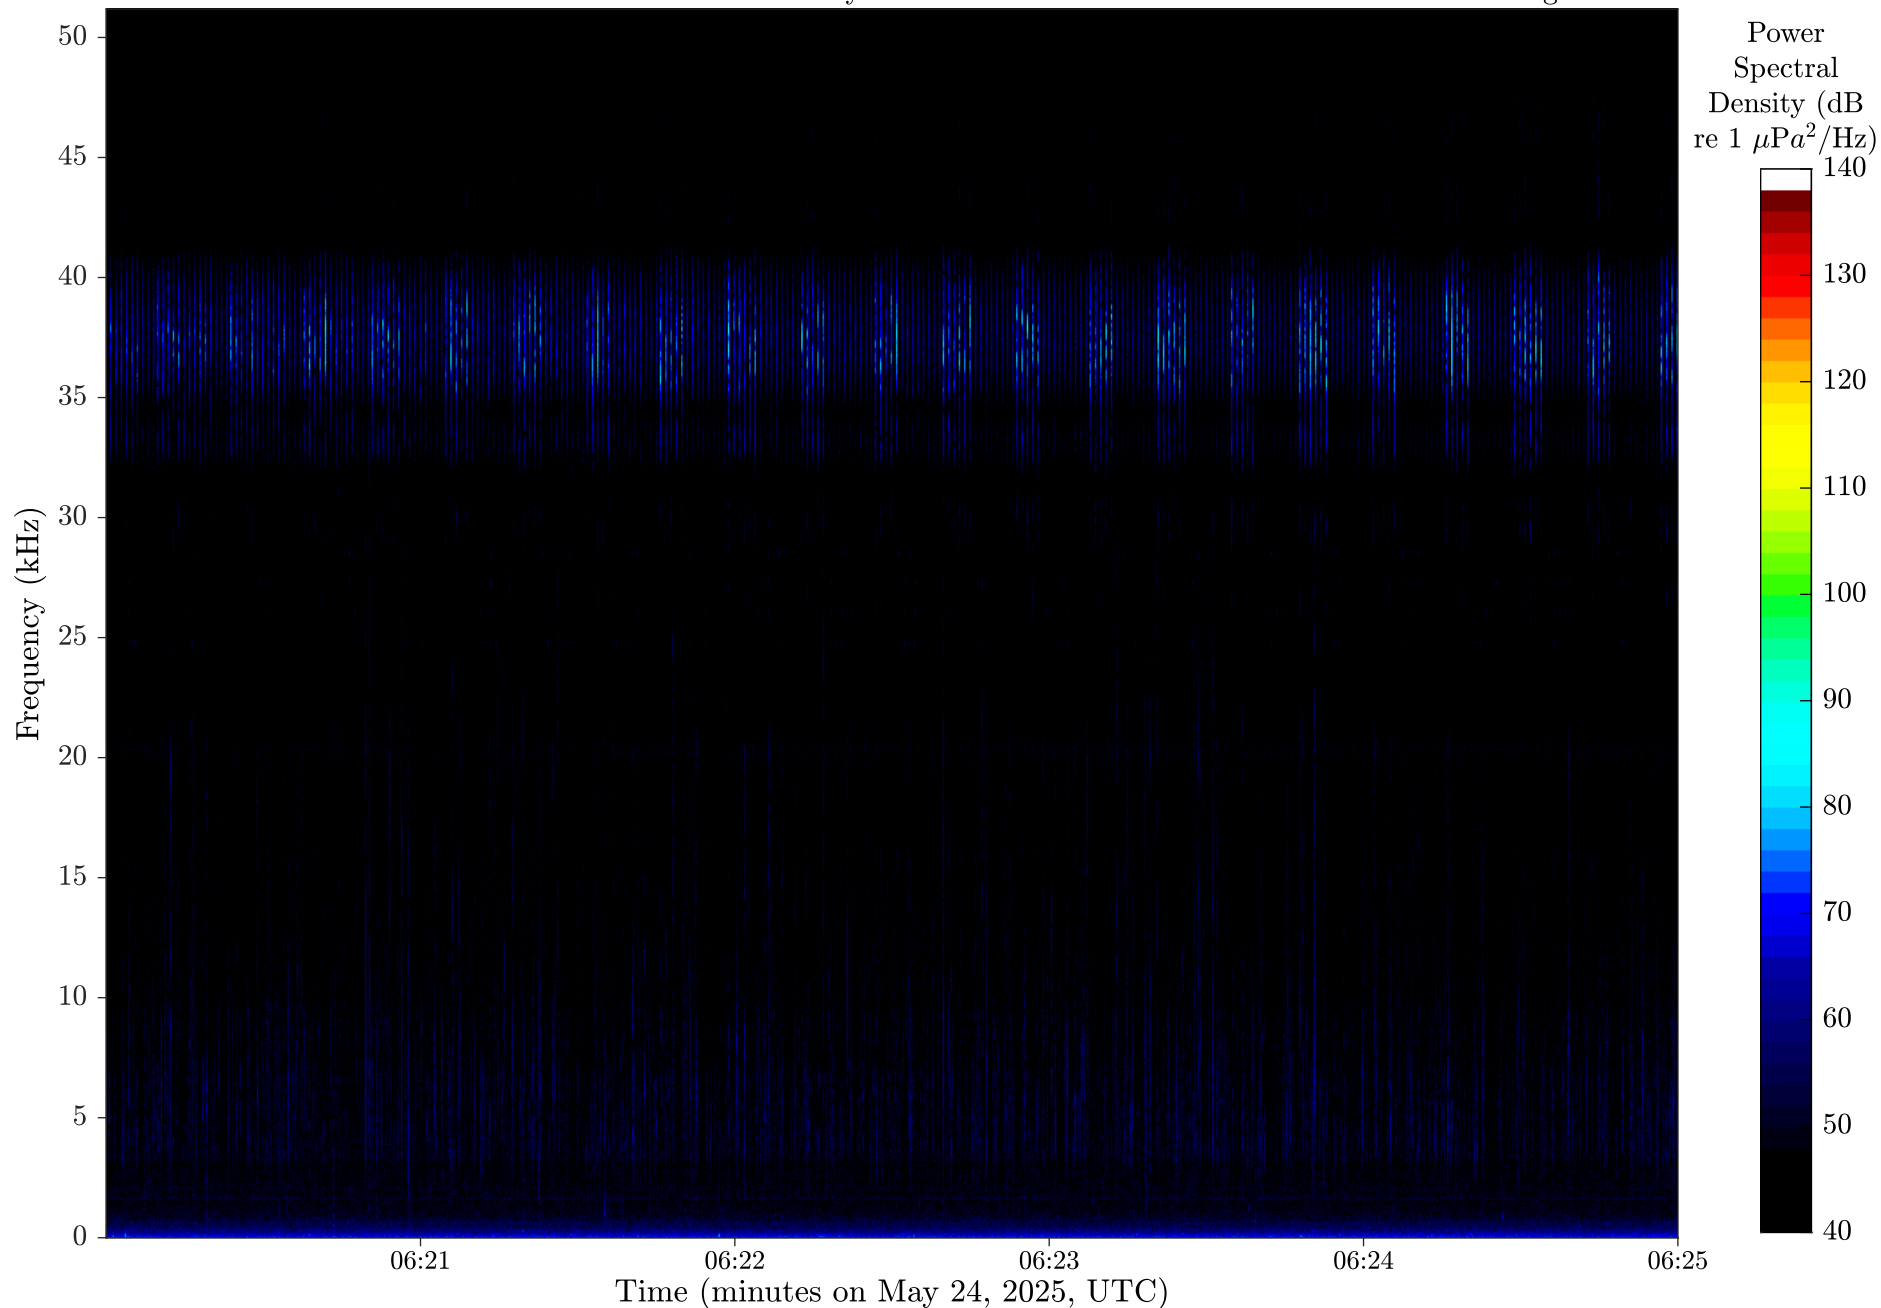


Comments: 35.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:40 UTC

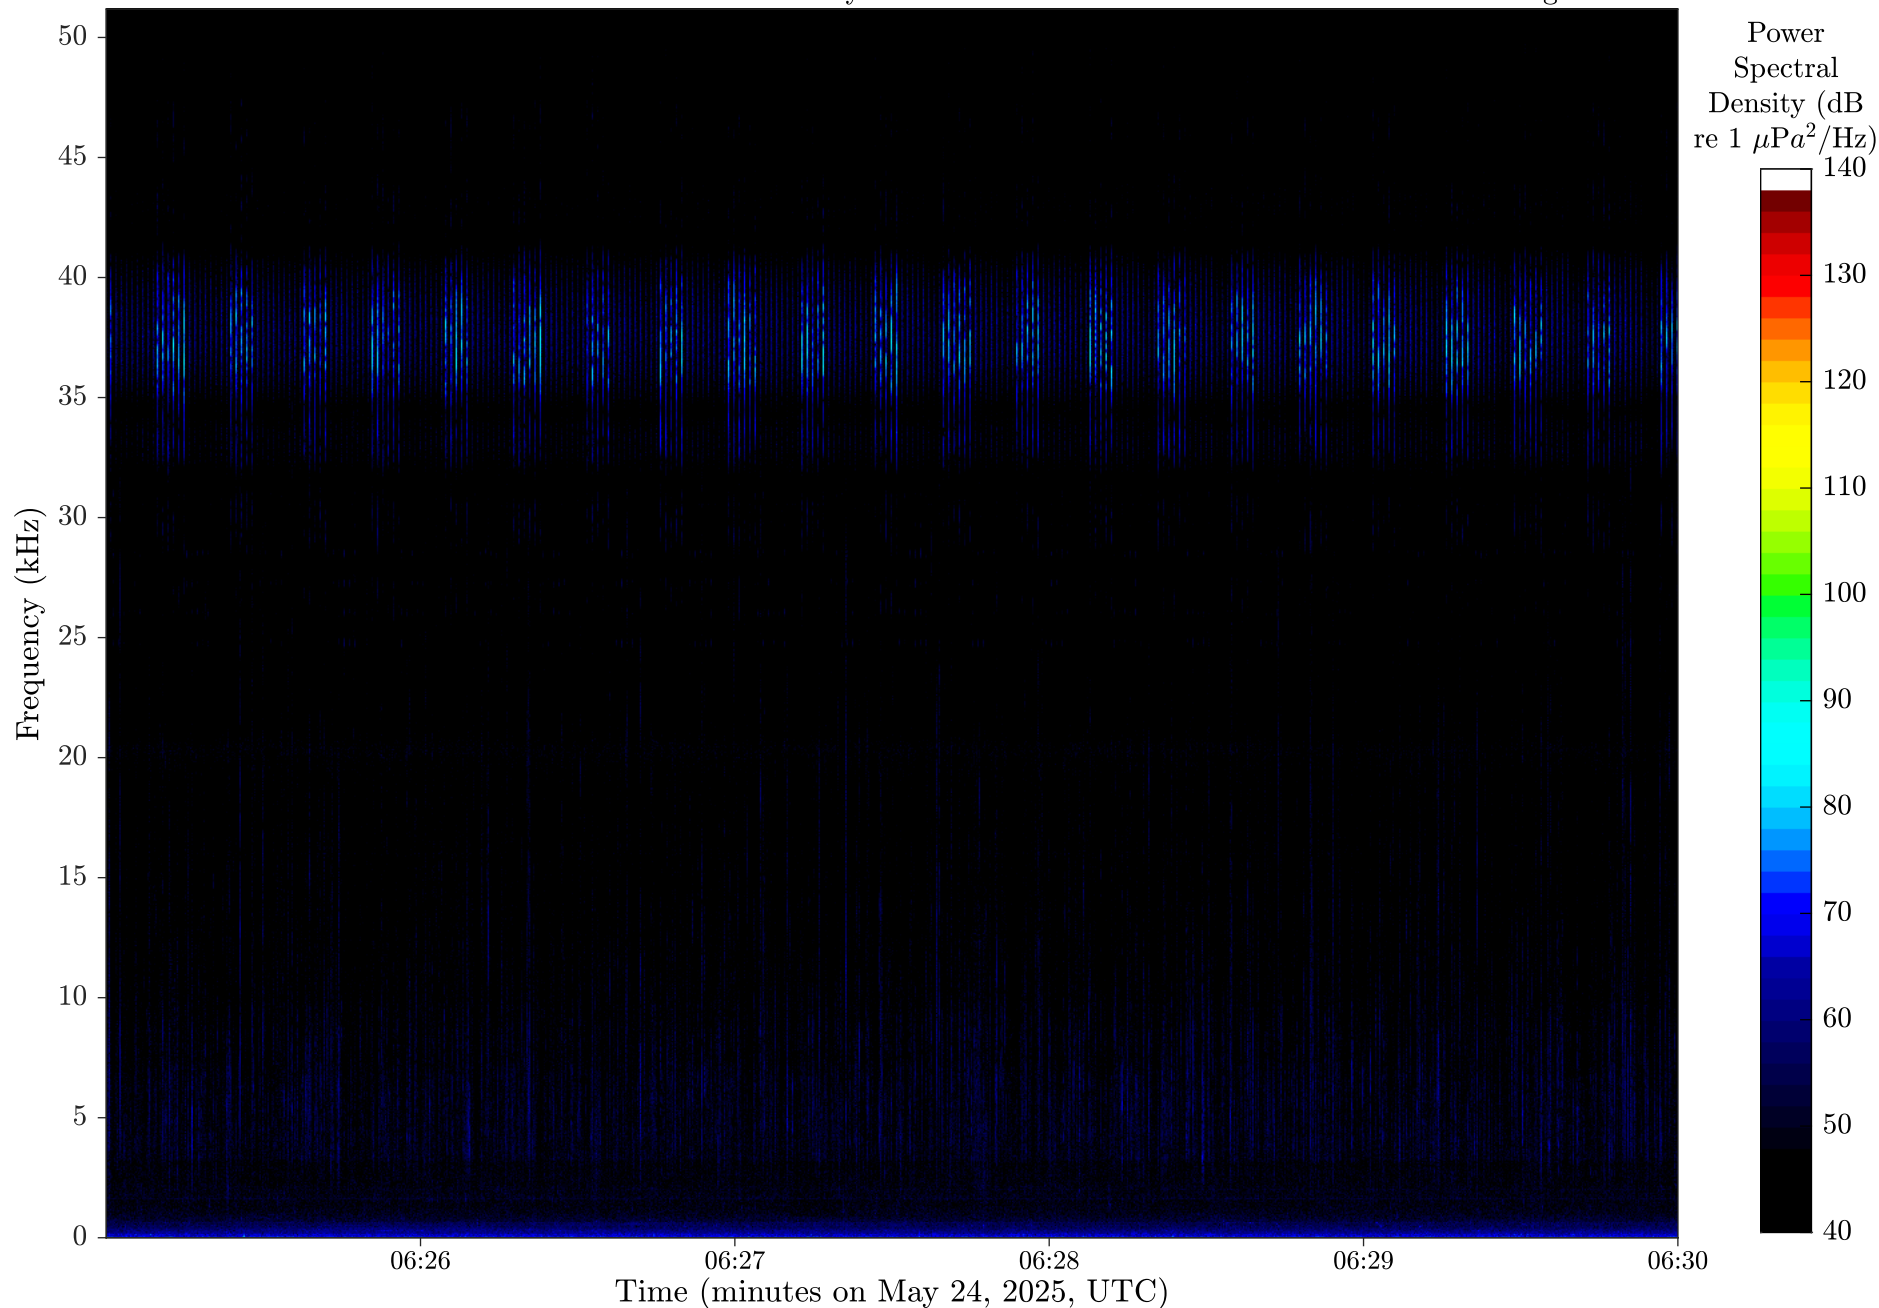


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:29:47 UTC

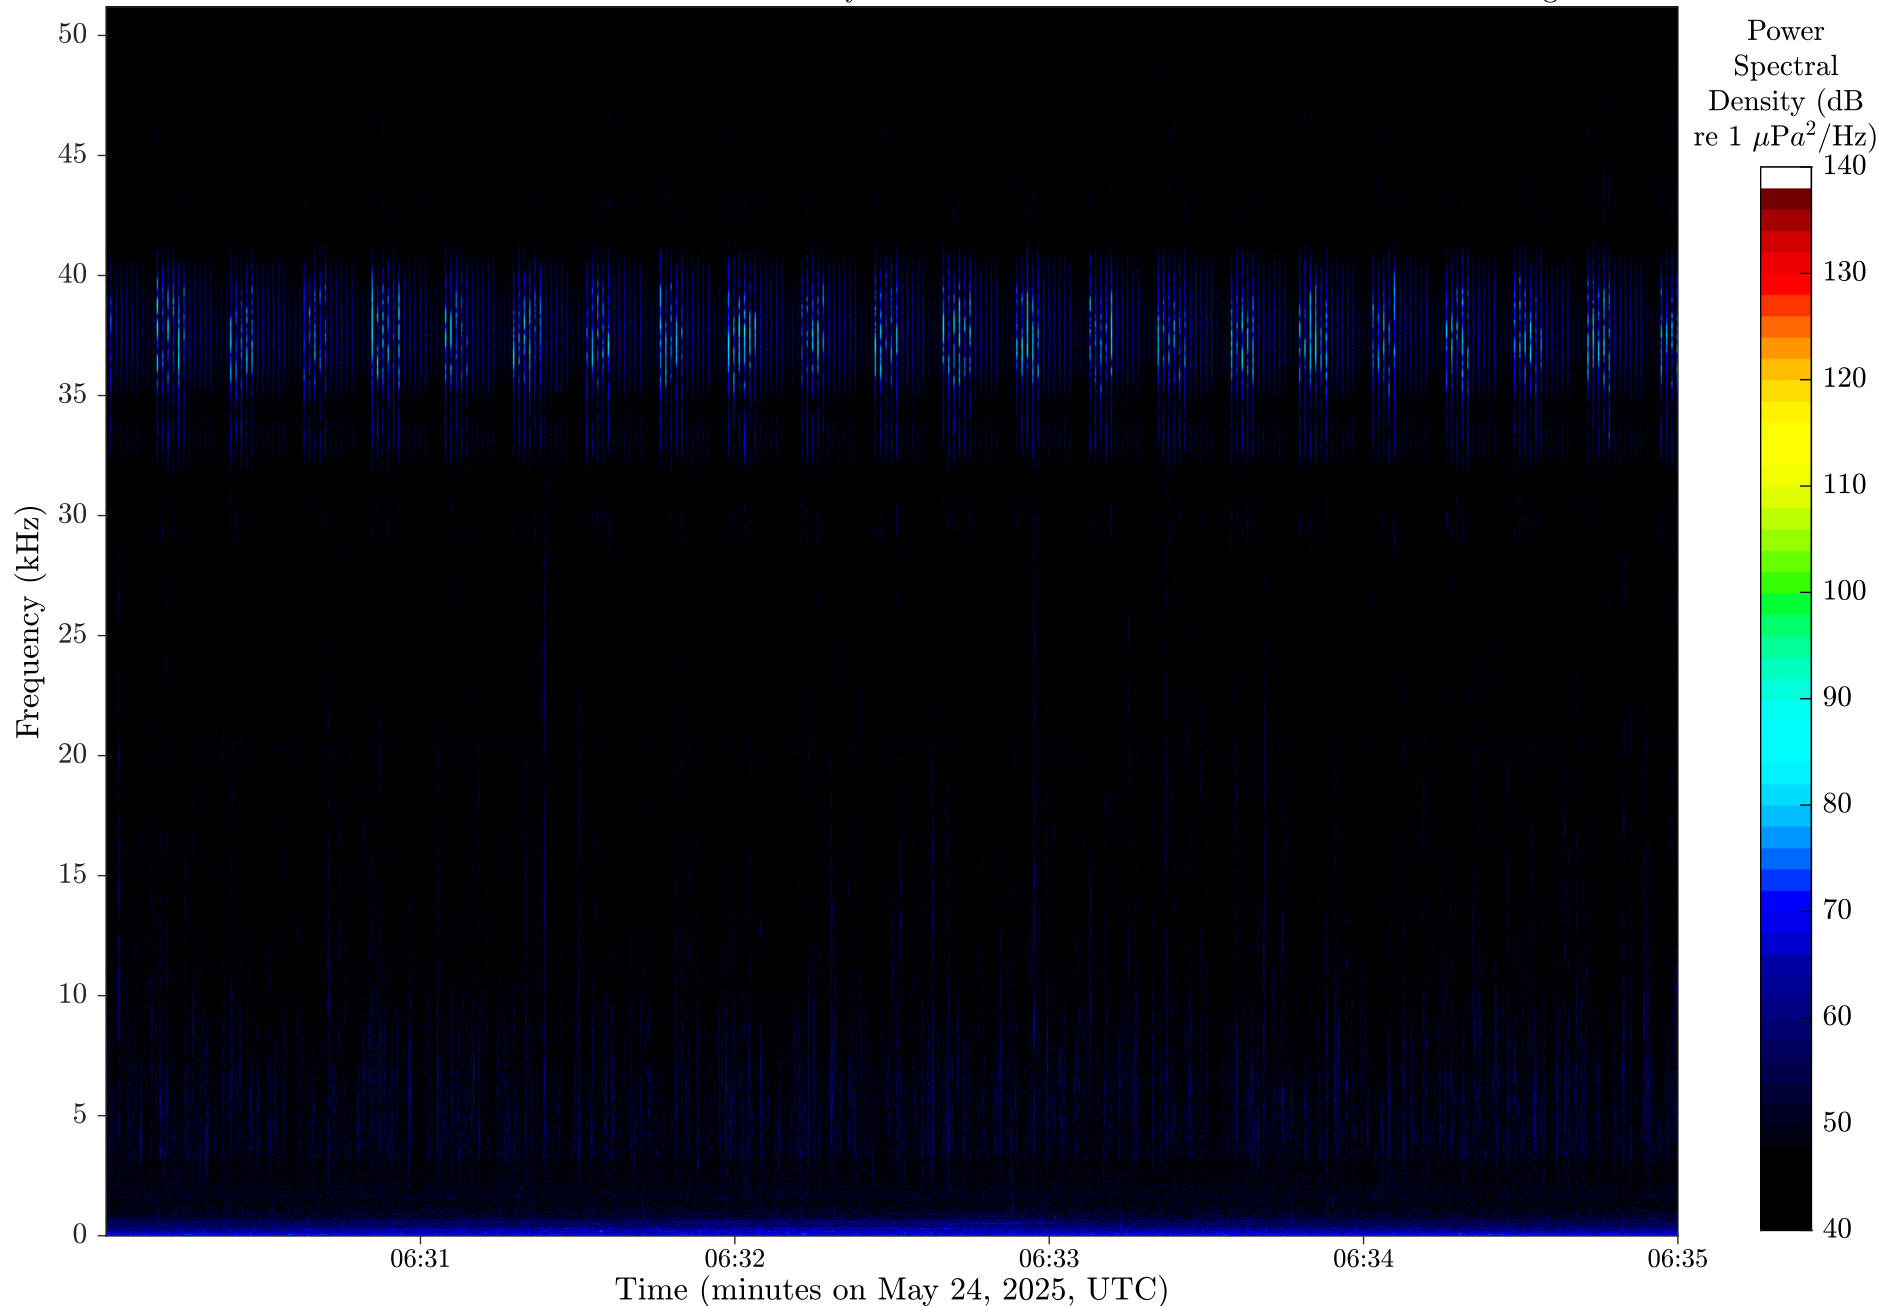


Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:29:55 UTC

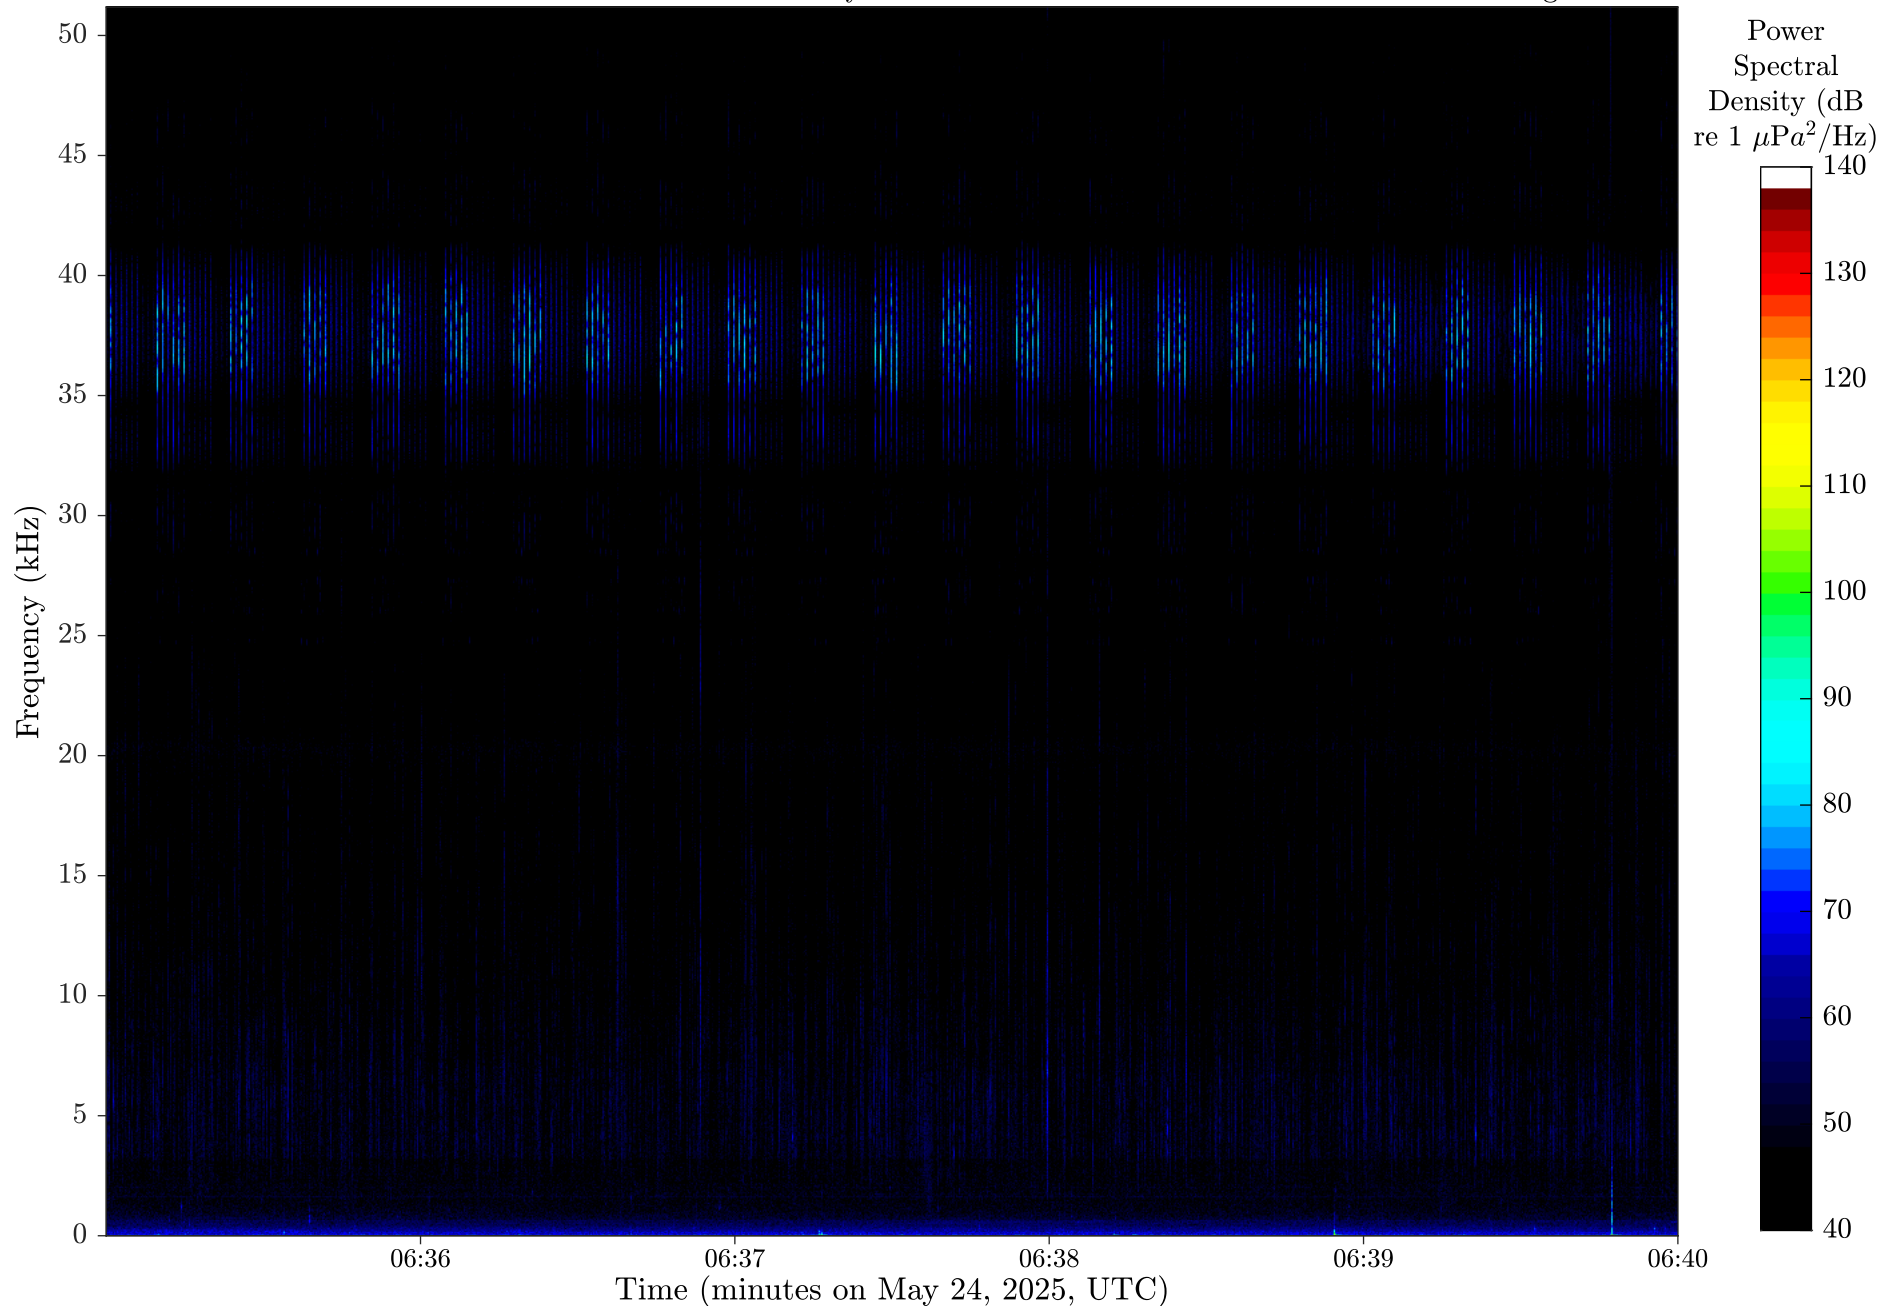

Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:30:04 UTC

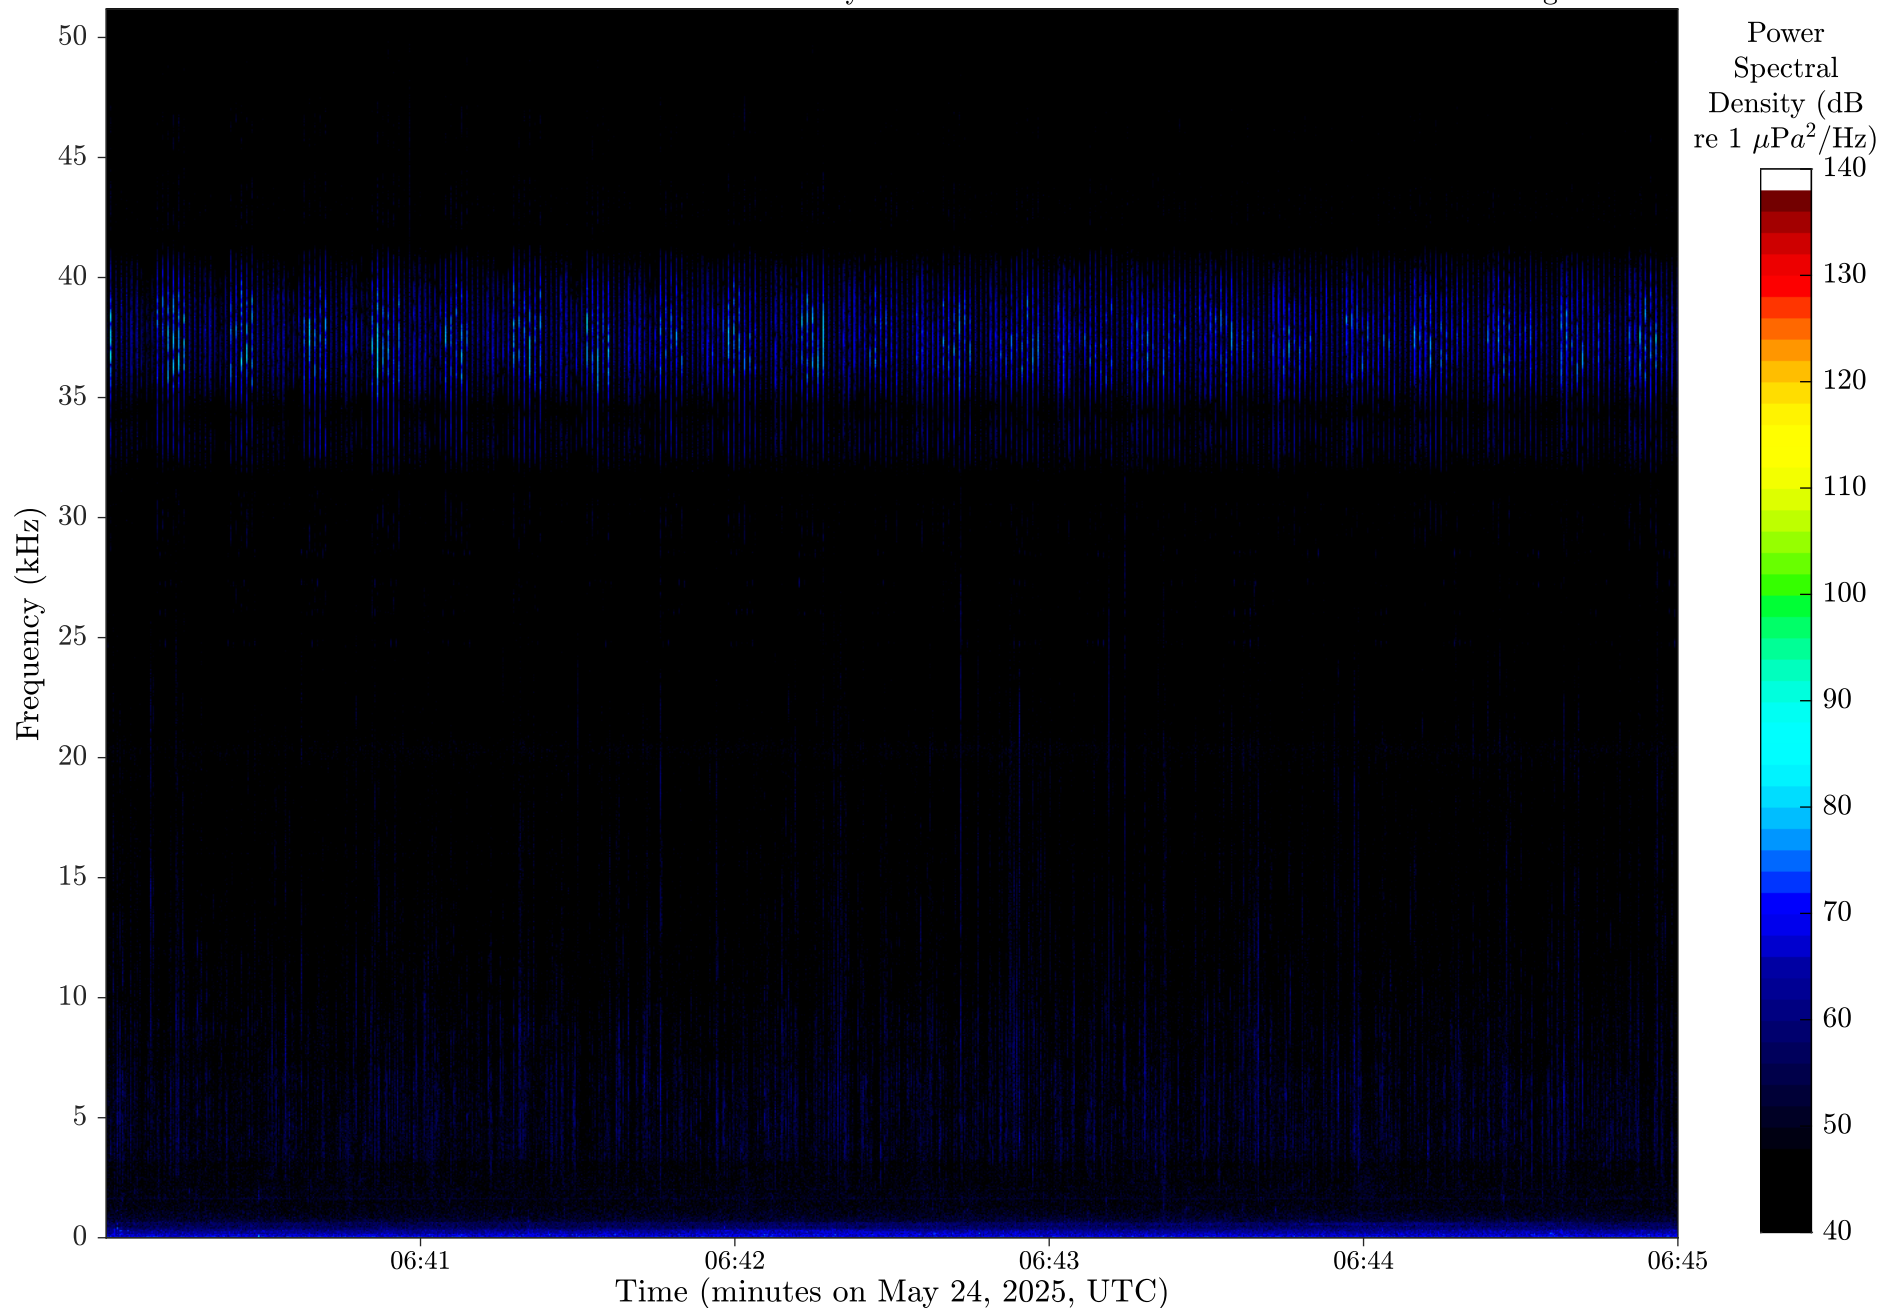


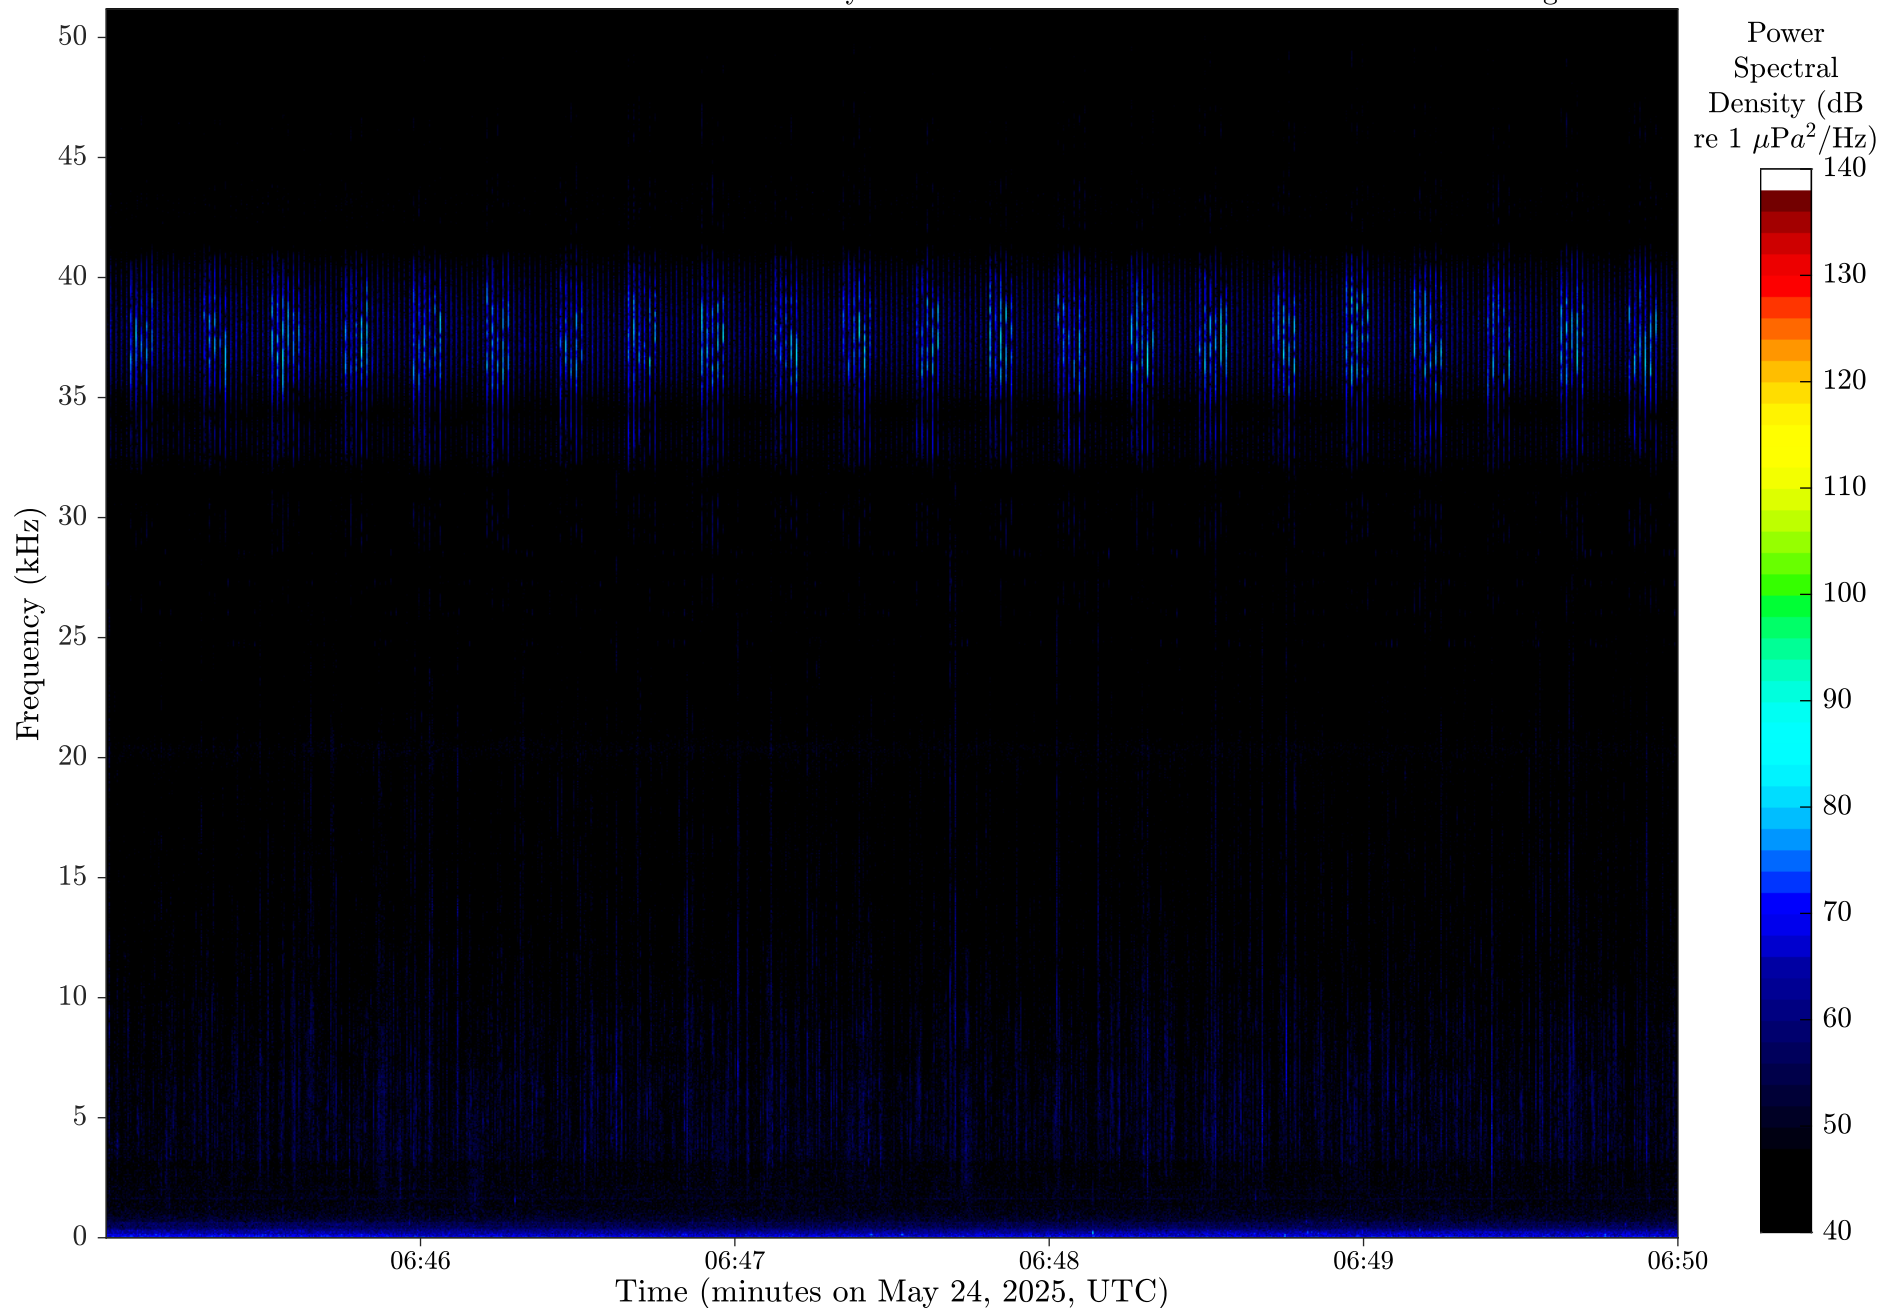

Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:30:20 UTC

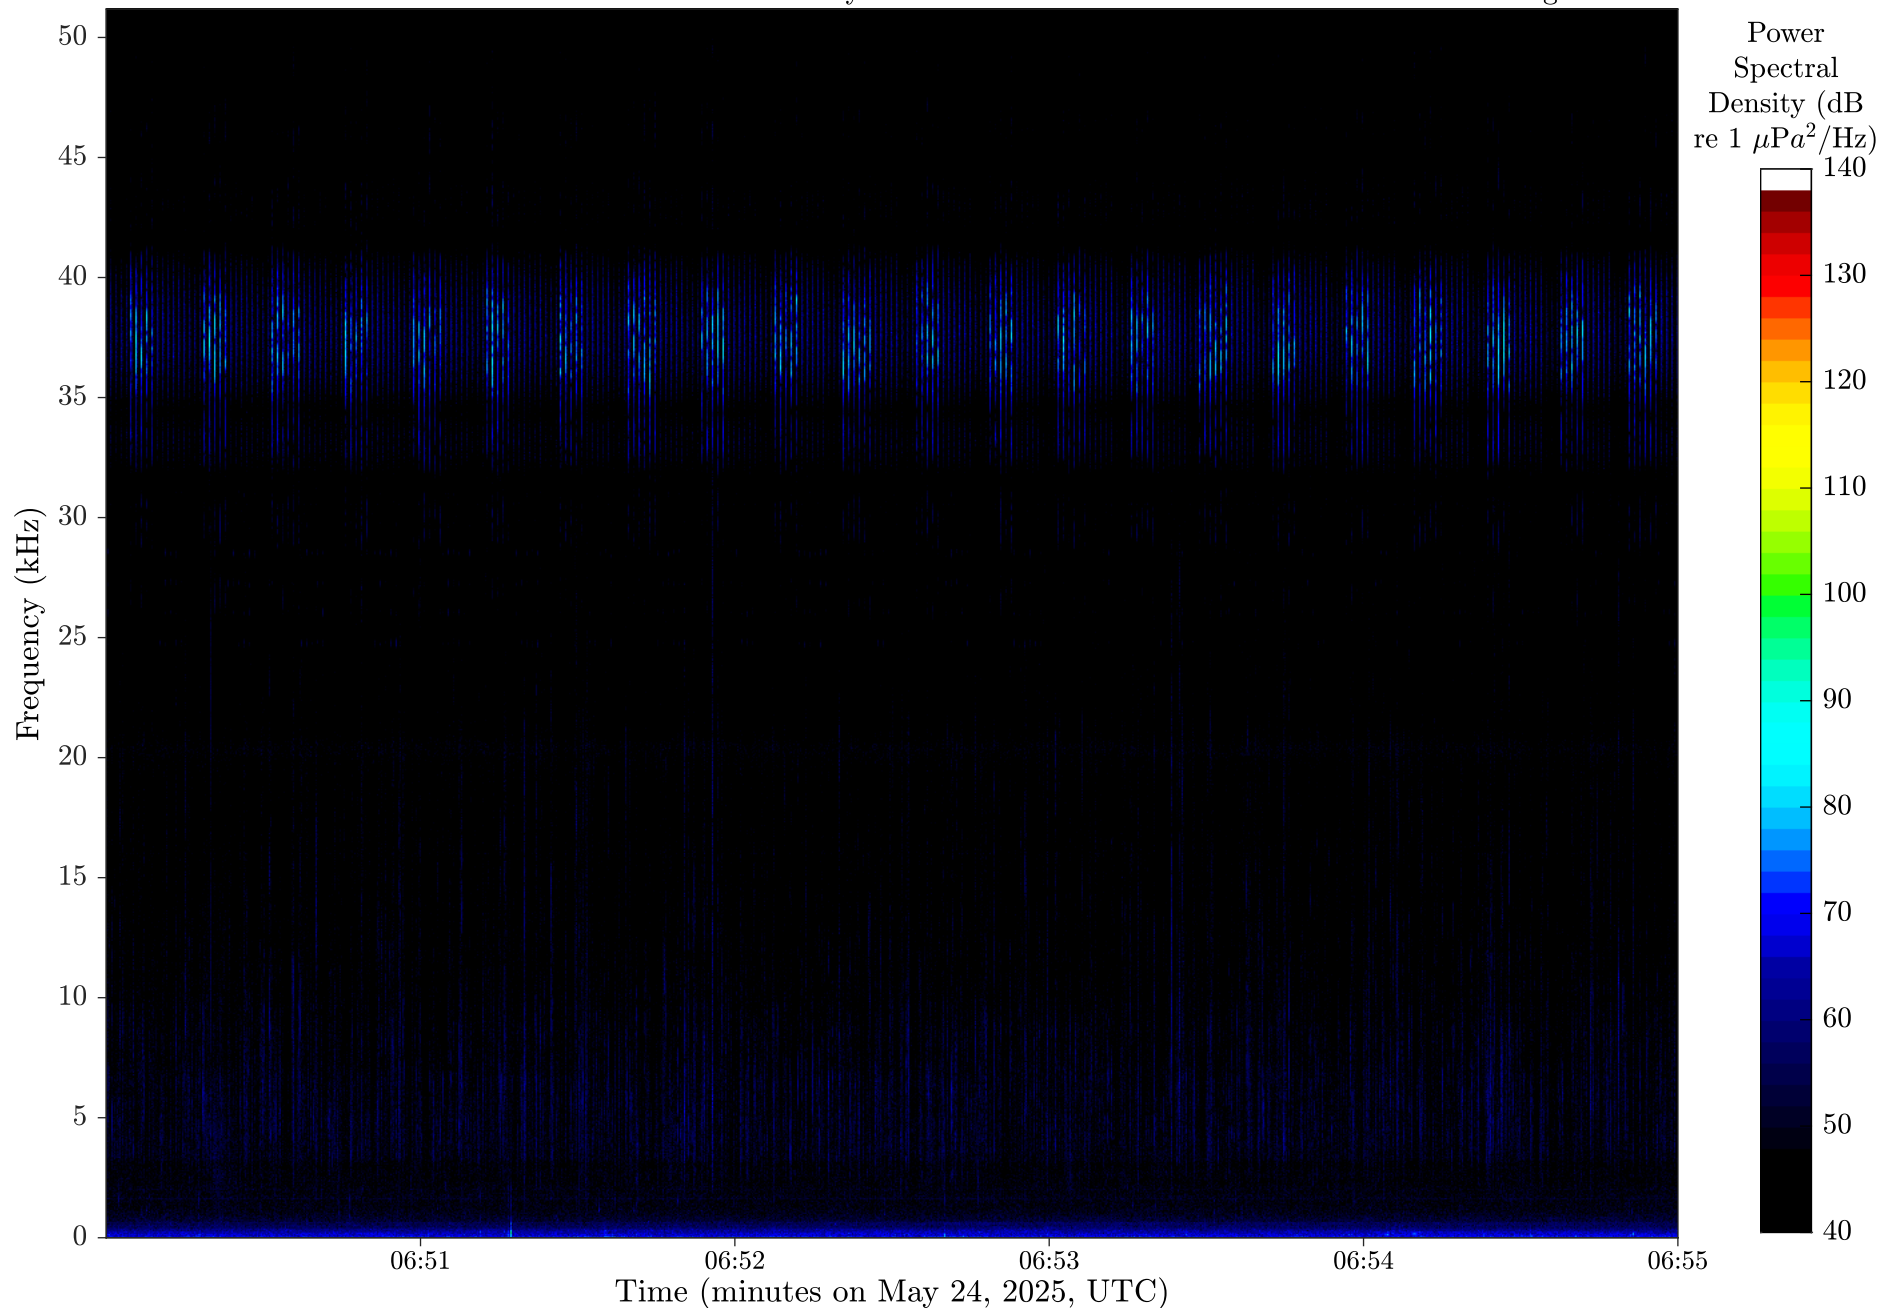

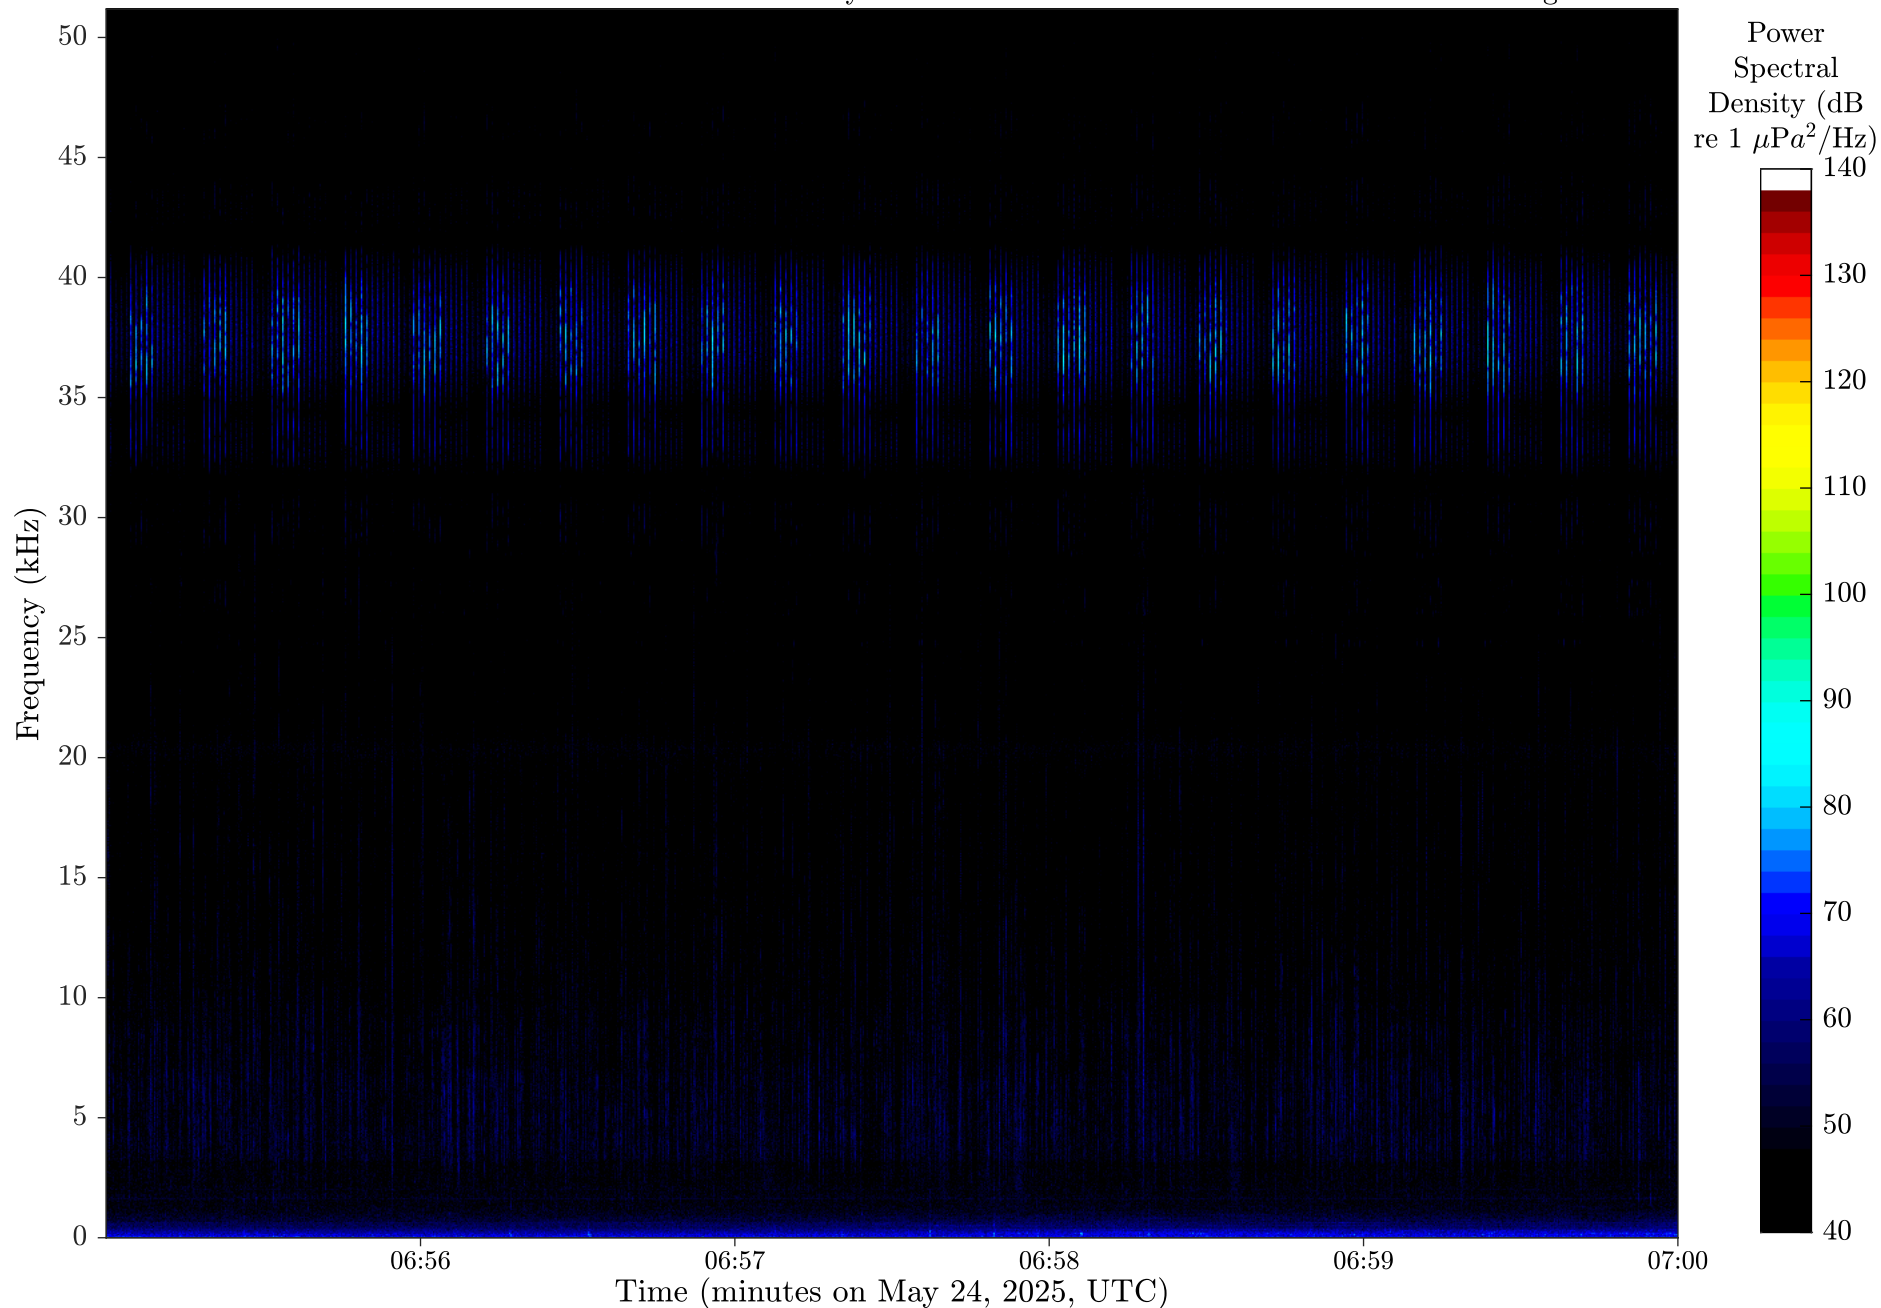


Comments: 36.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:30:36 UTC

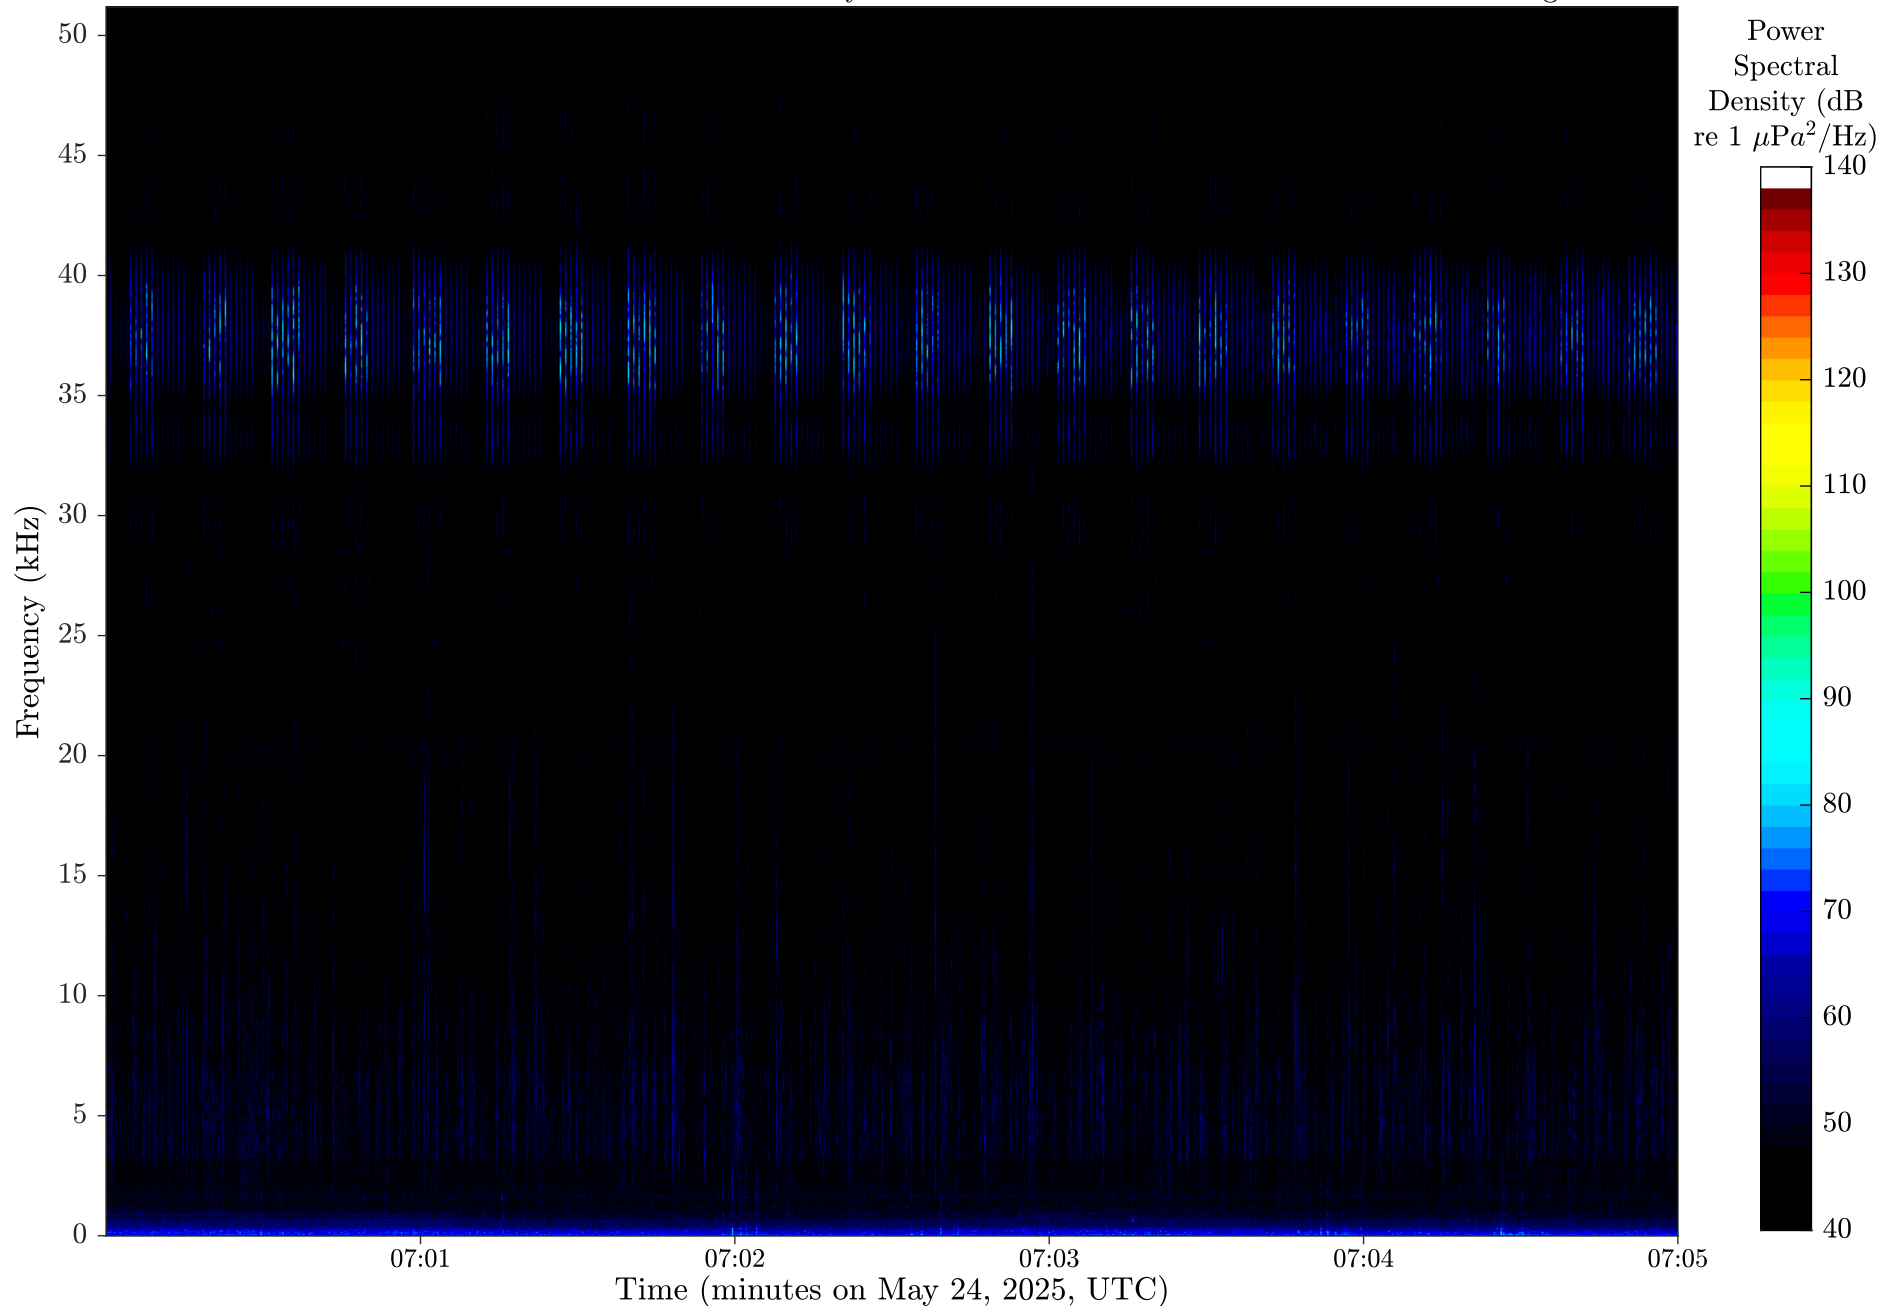


Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:30:44 UTC

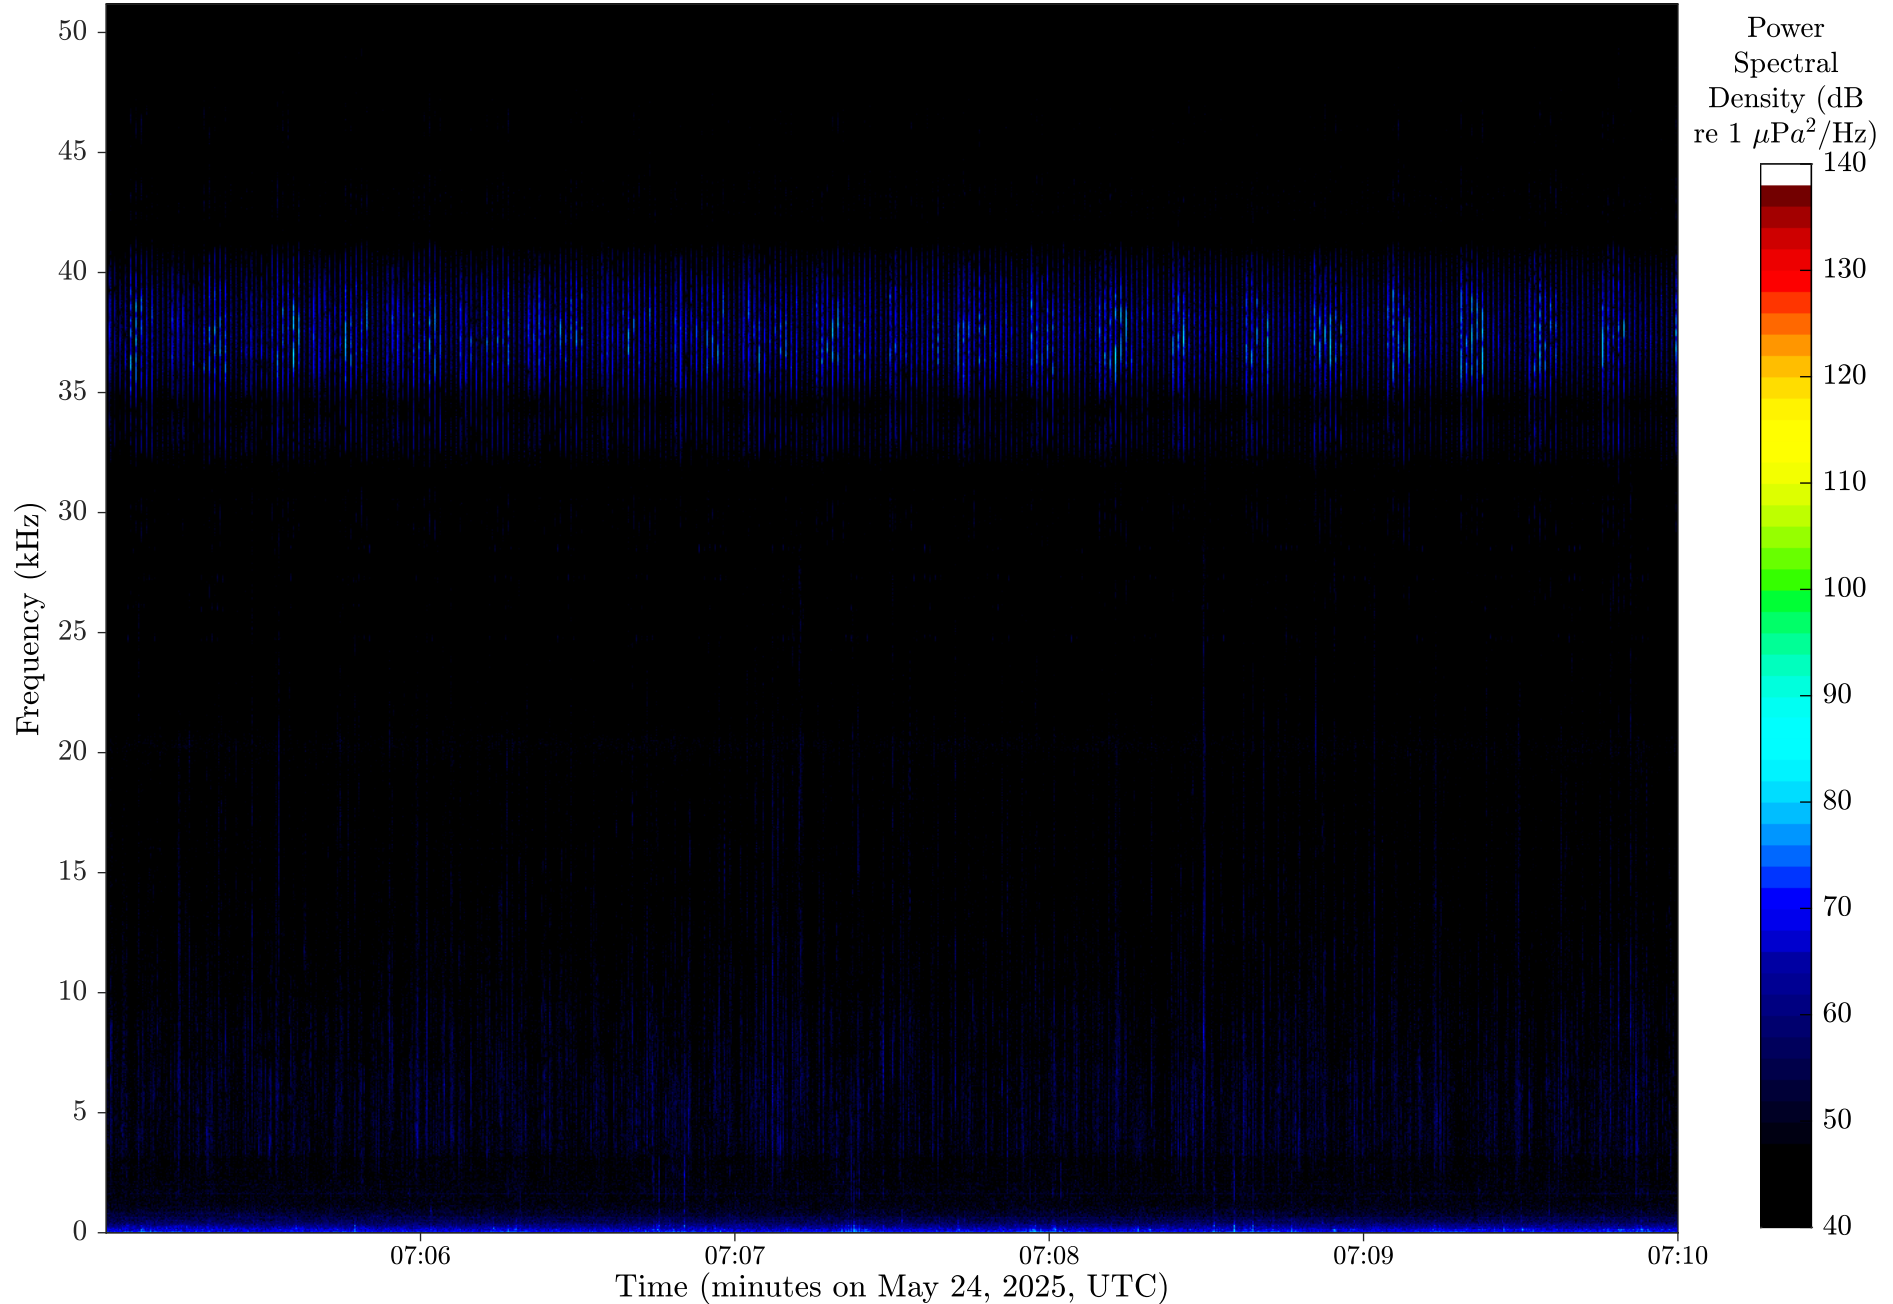


Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:30:53 UTC

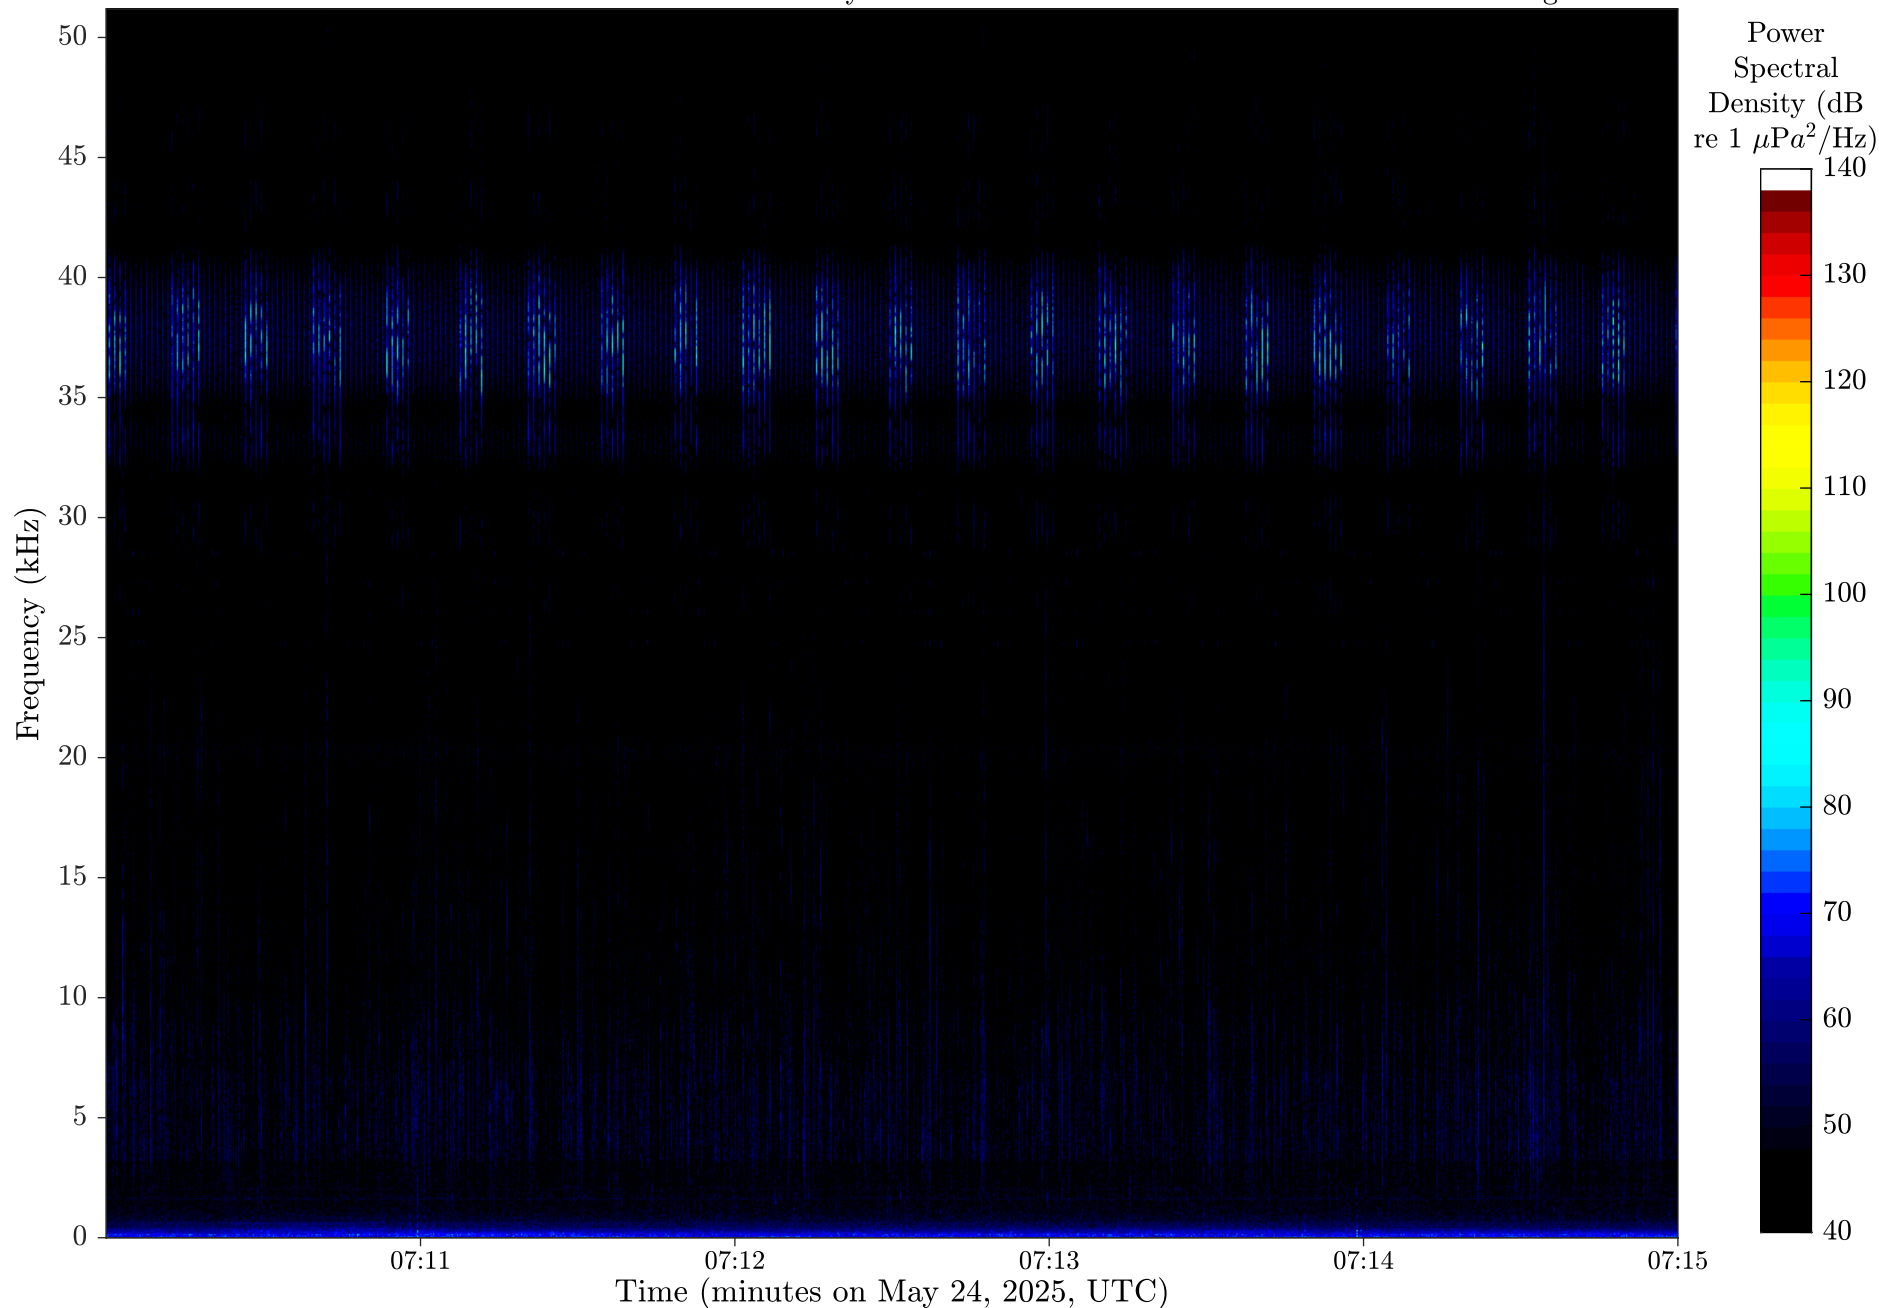


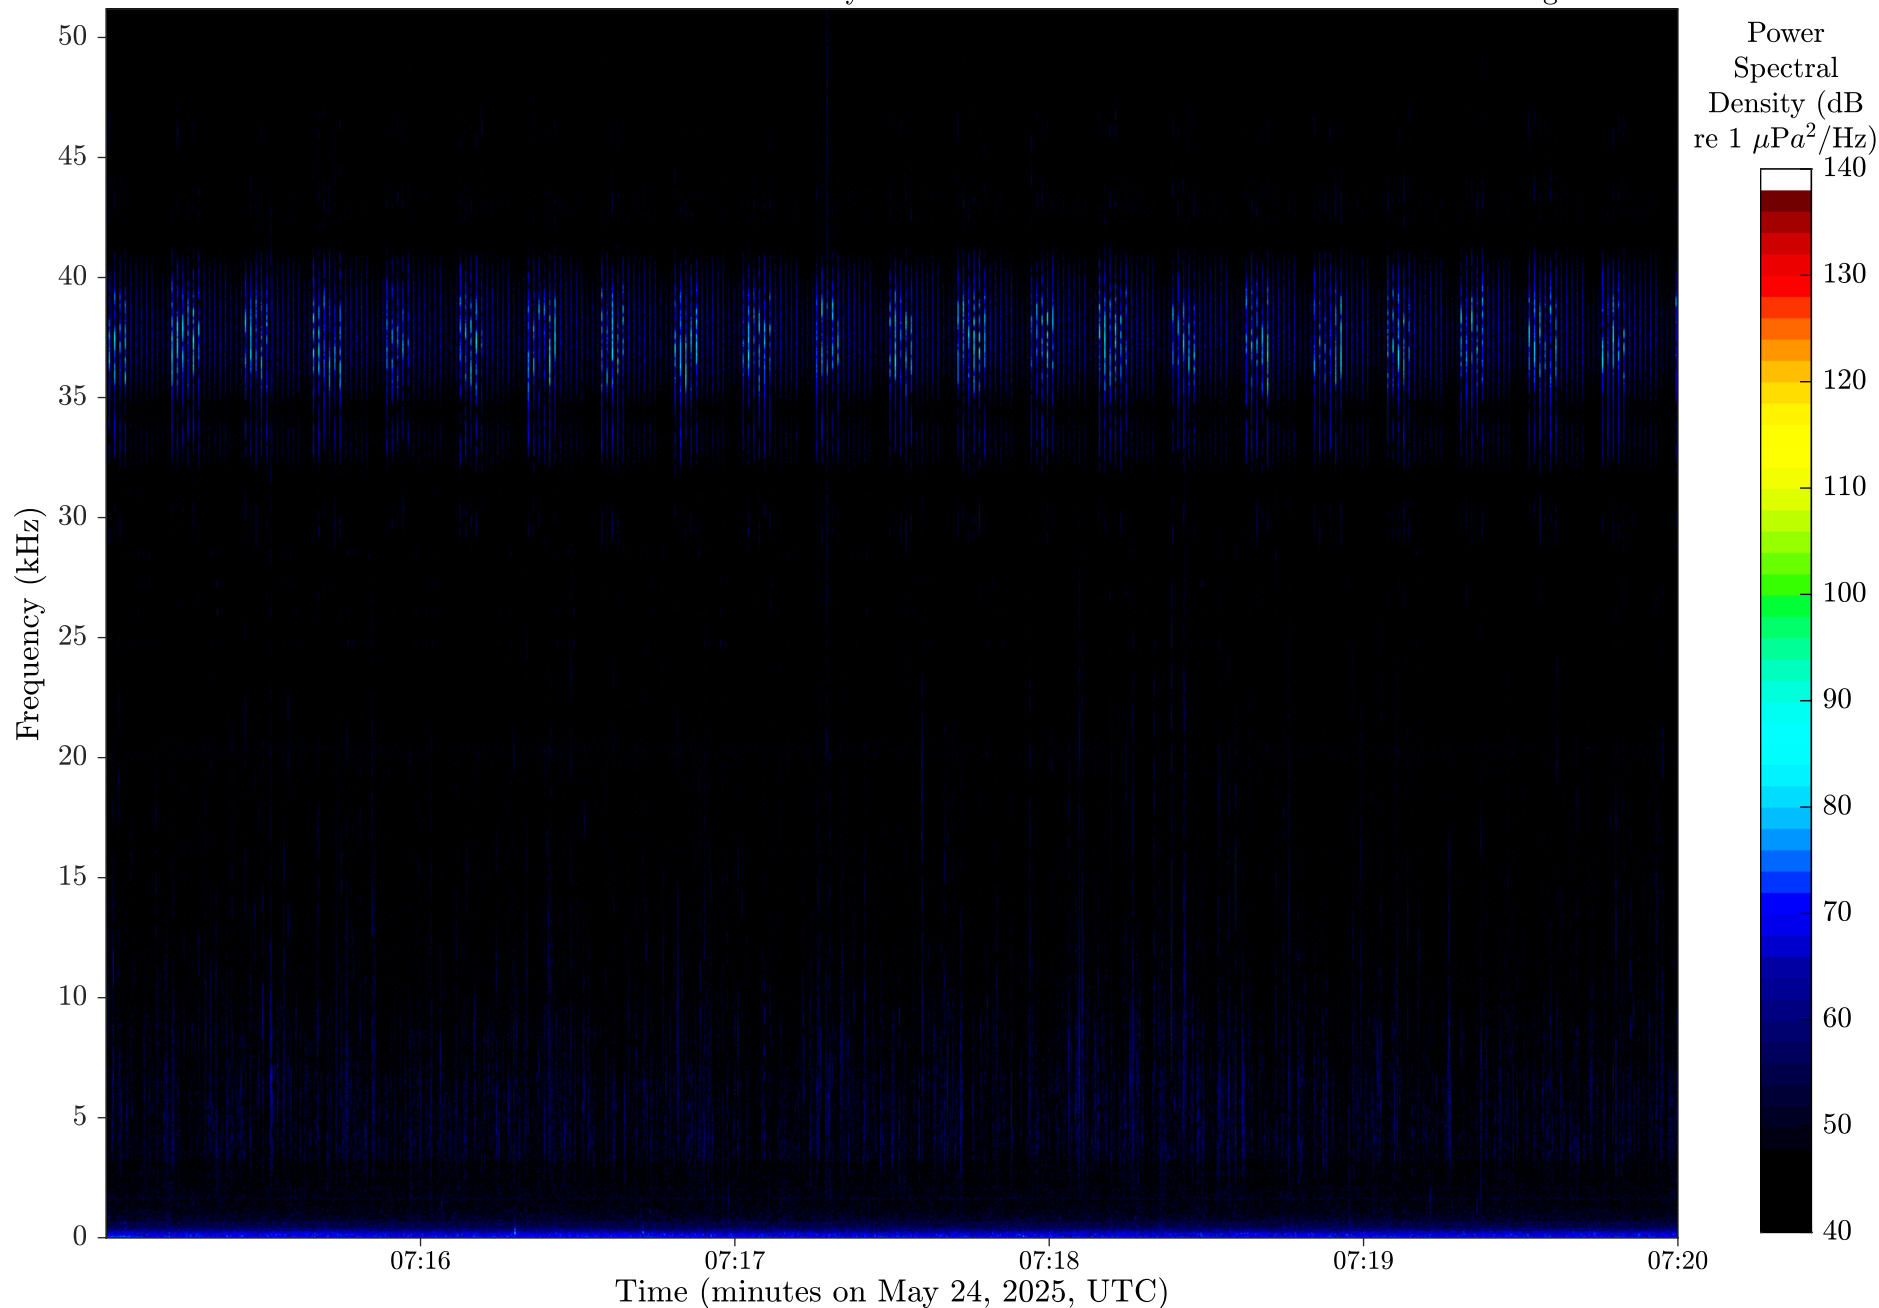


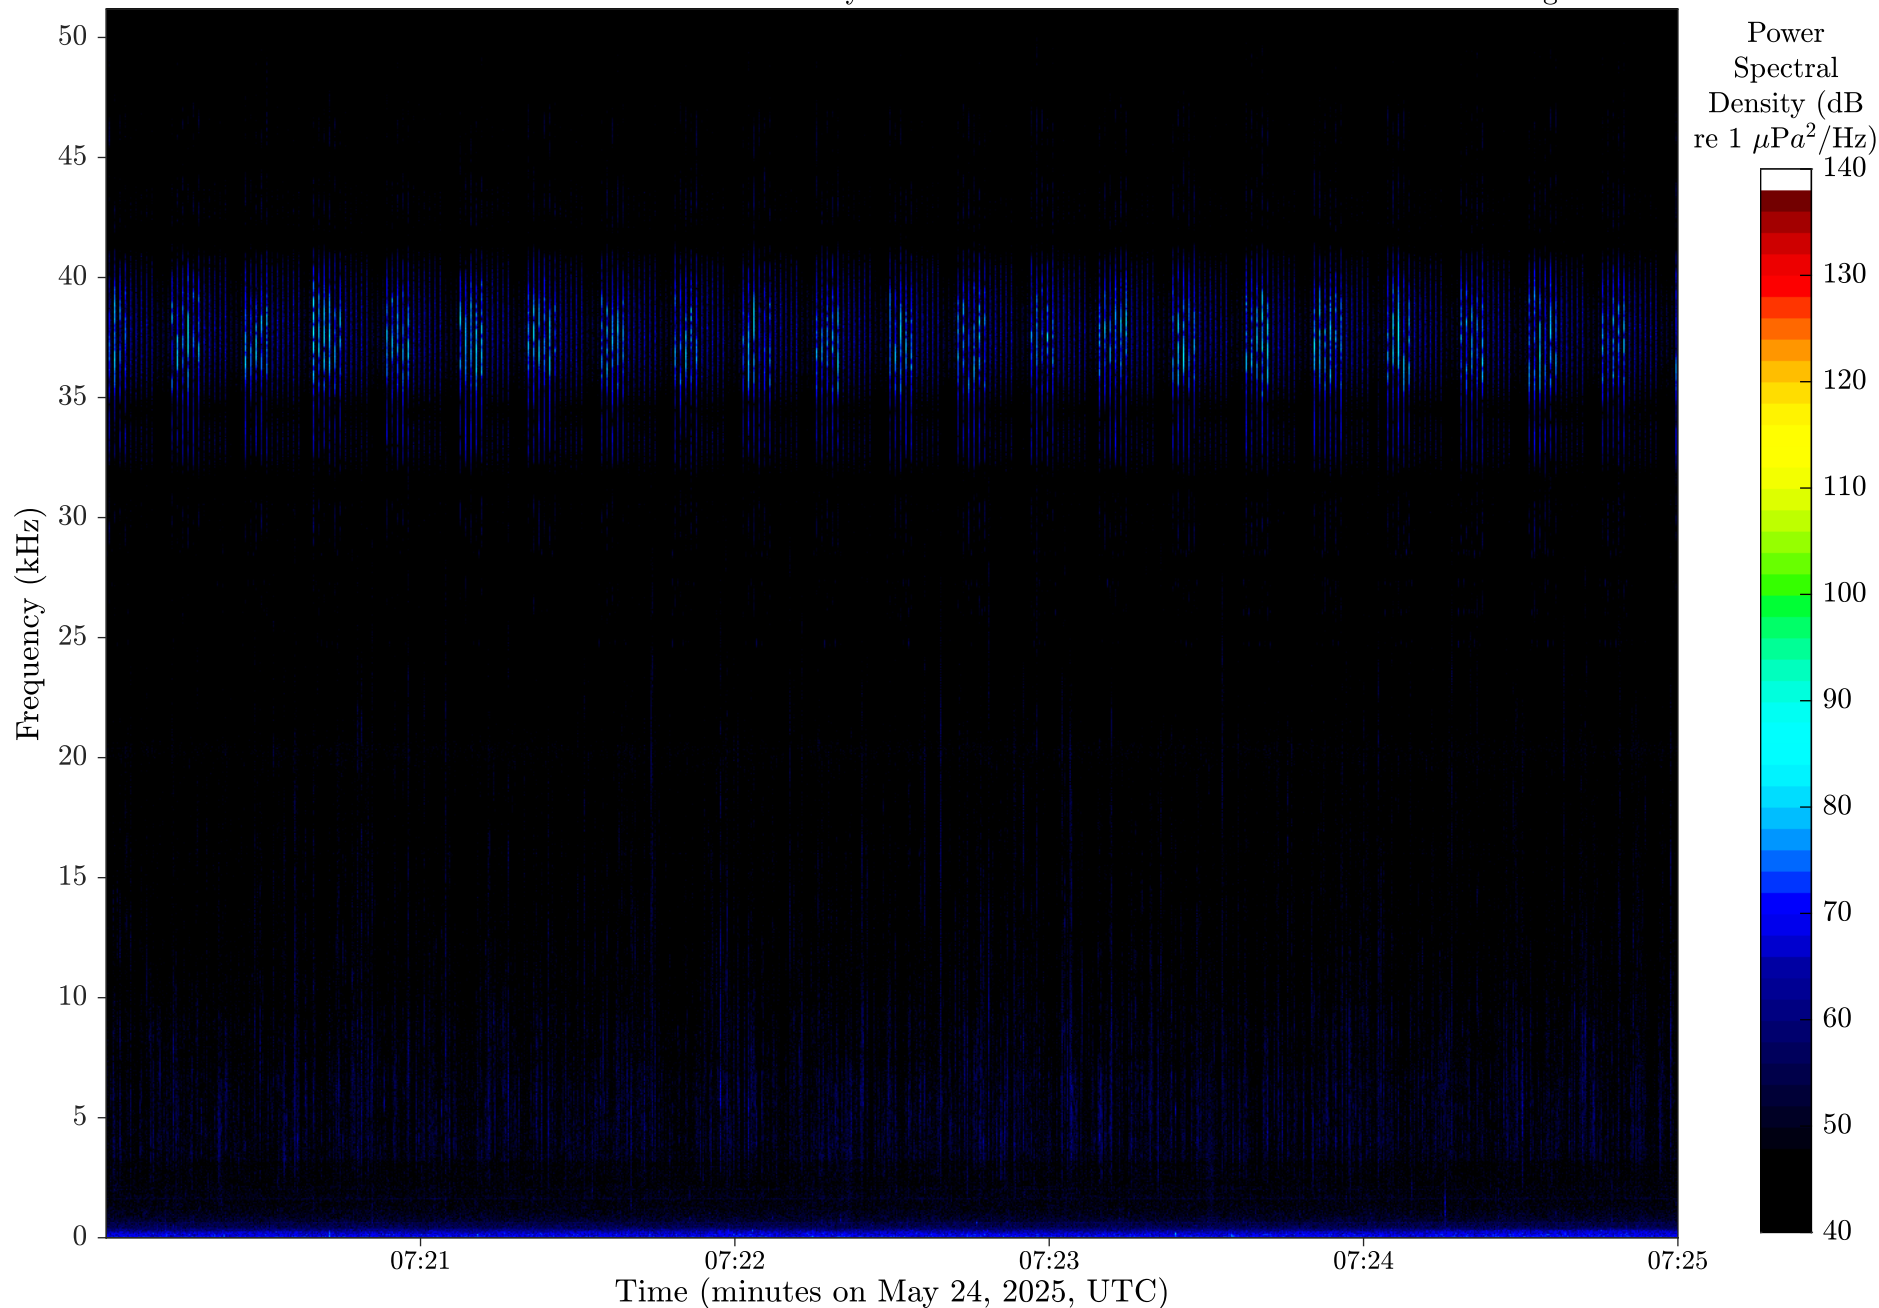

Comments: 36.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:31:19 UTC

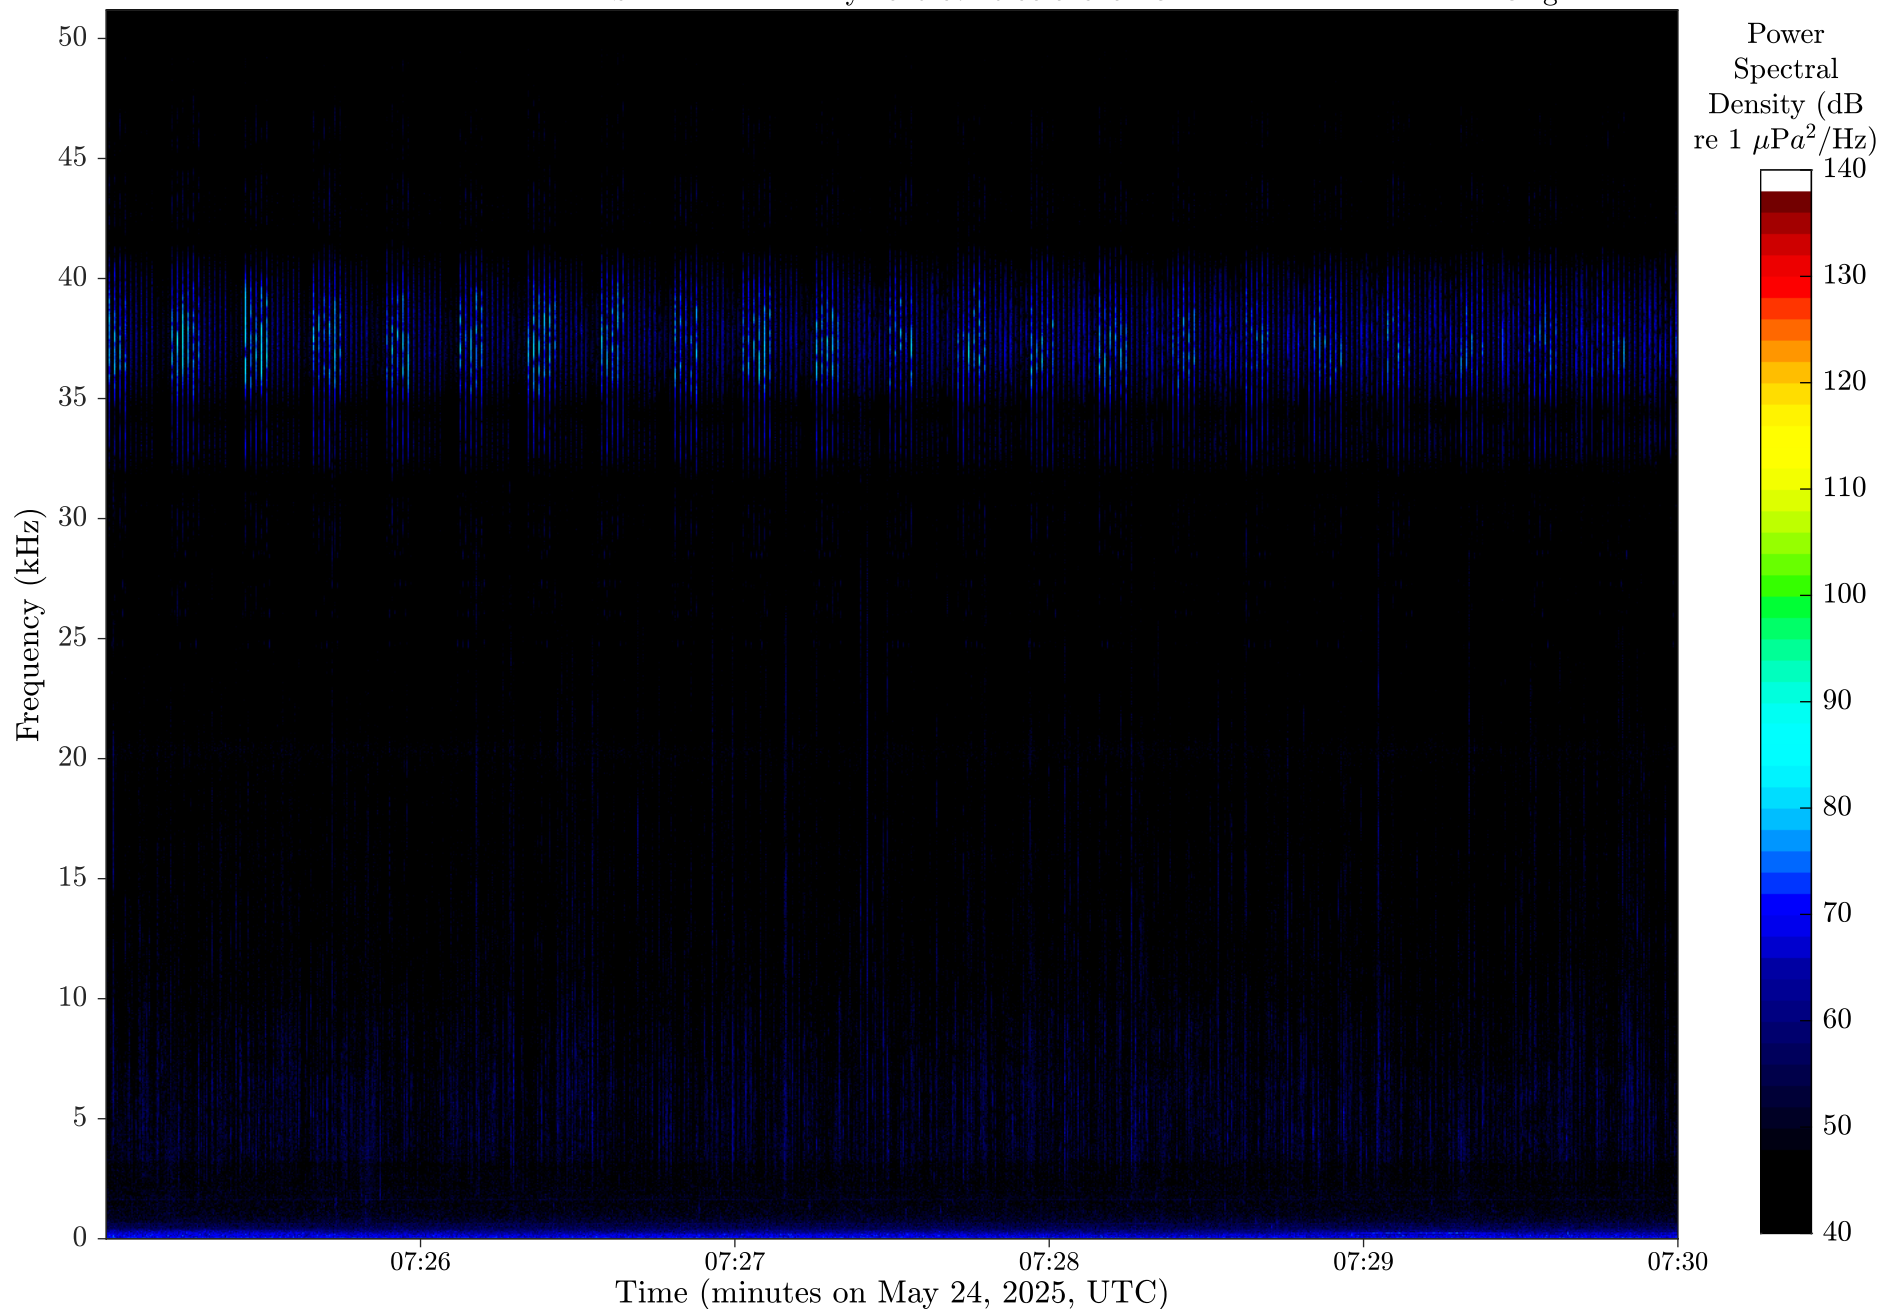


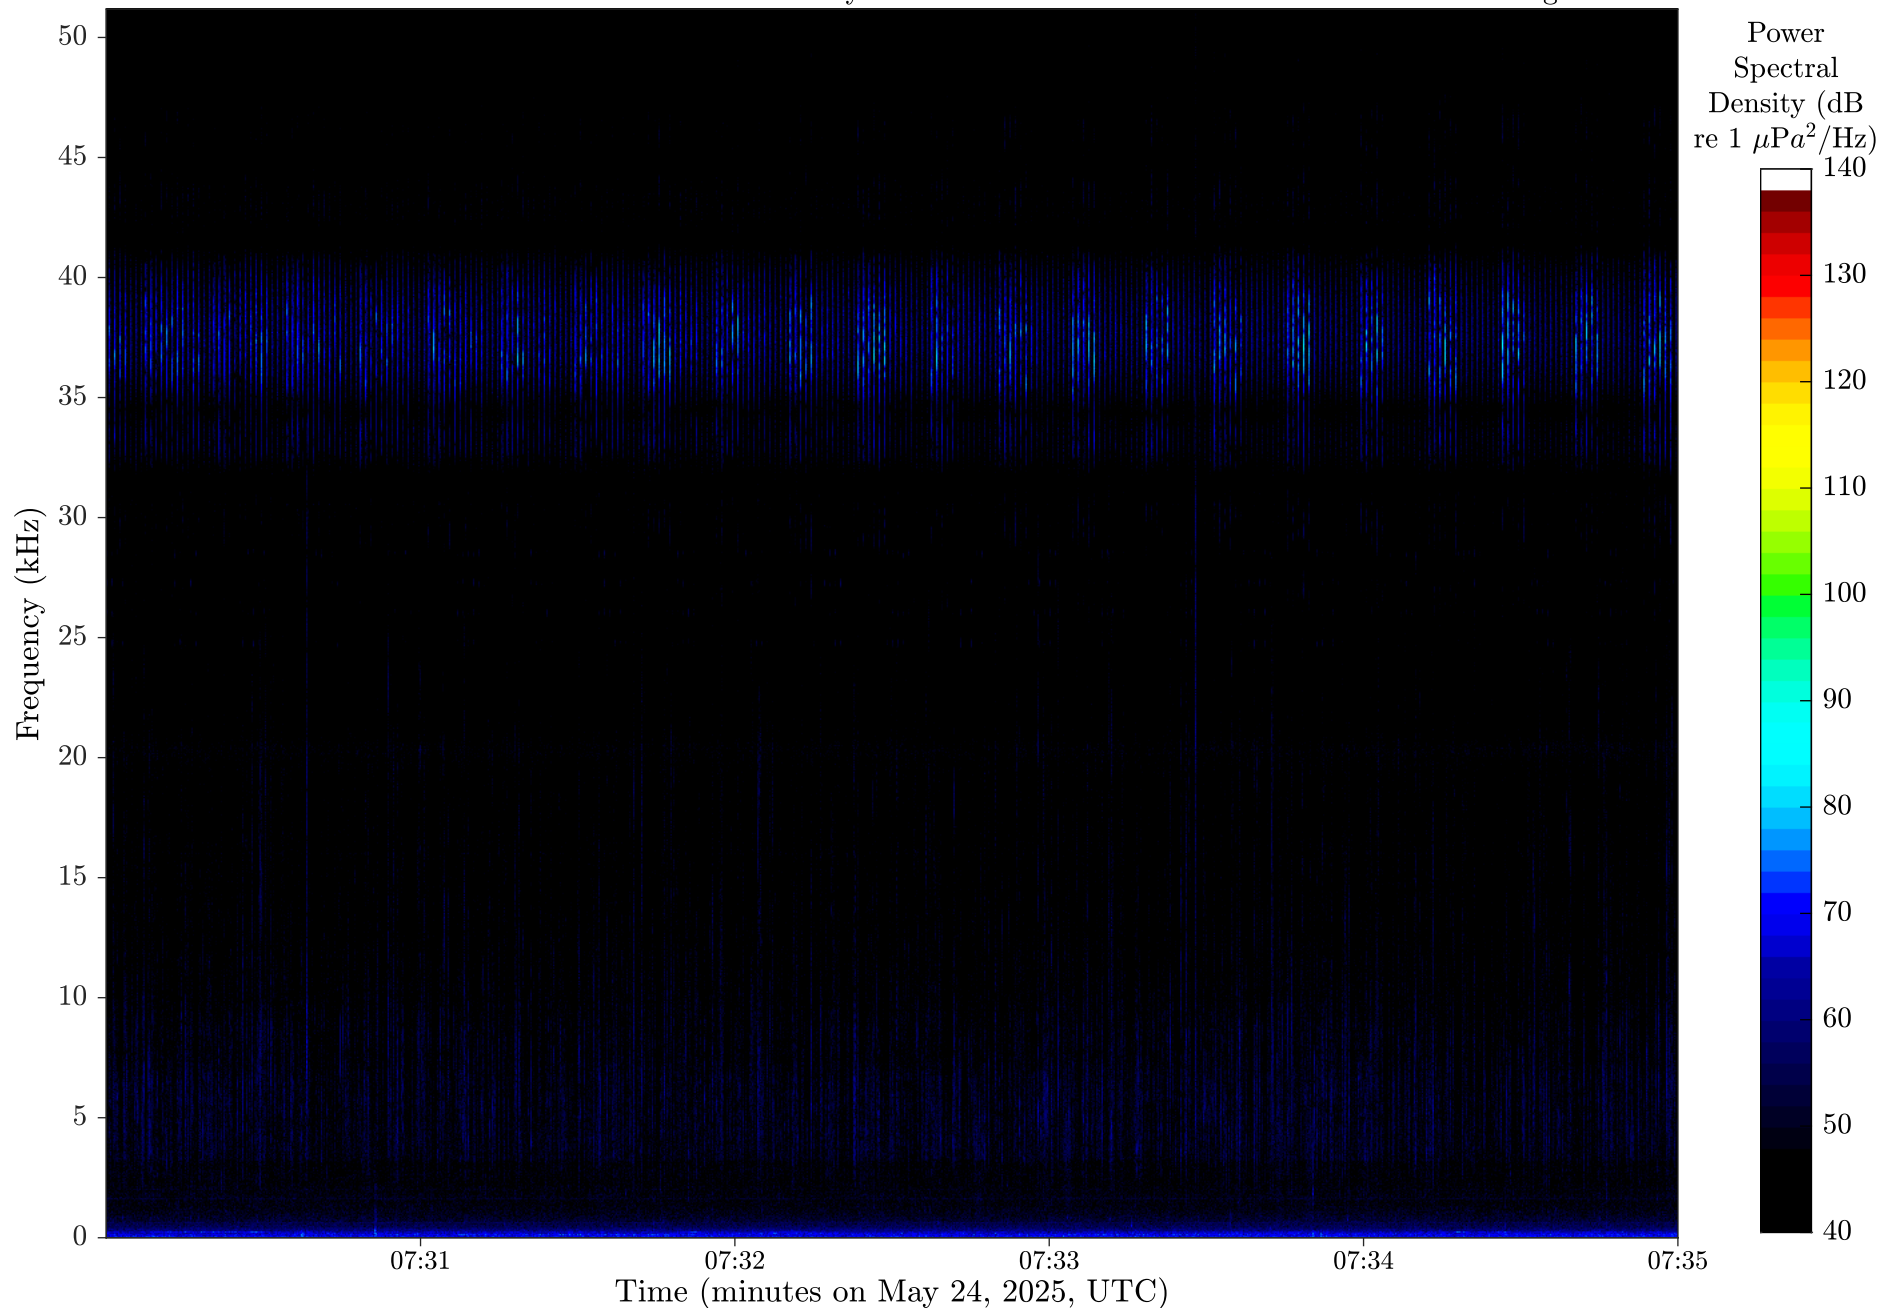

Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:31:36 UTC

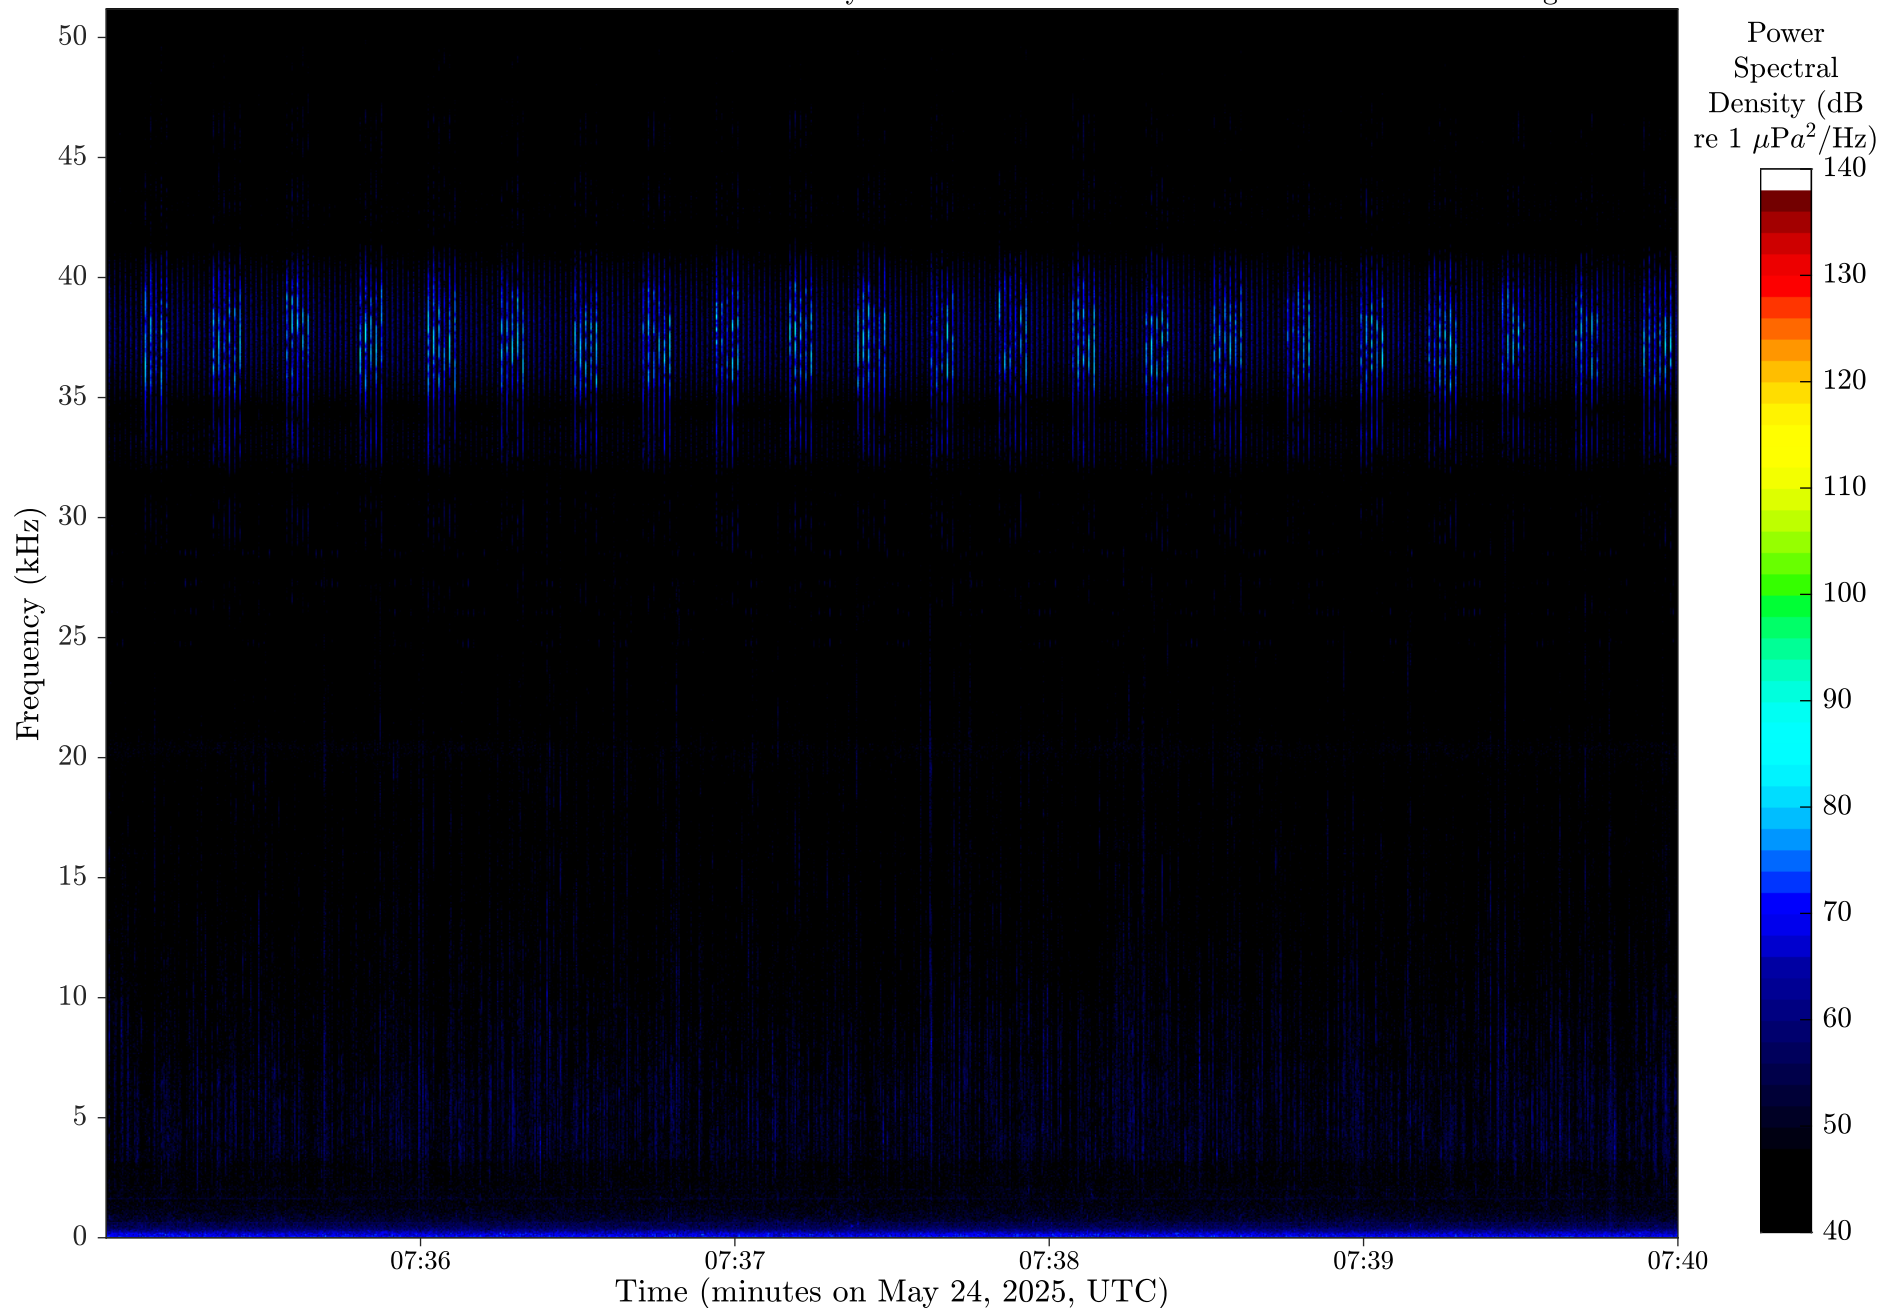

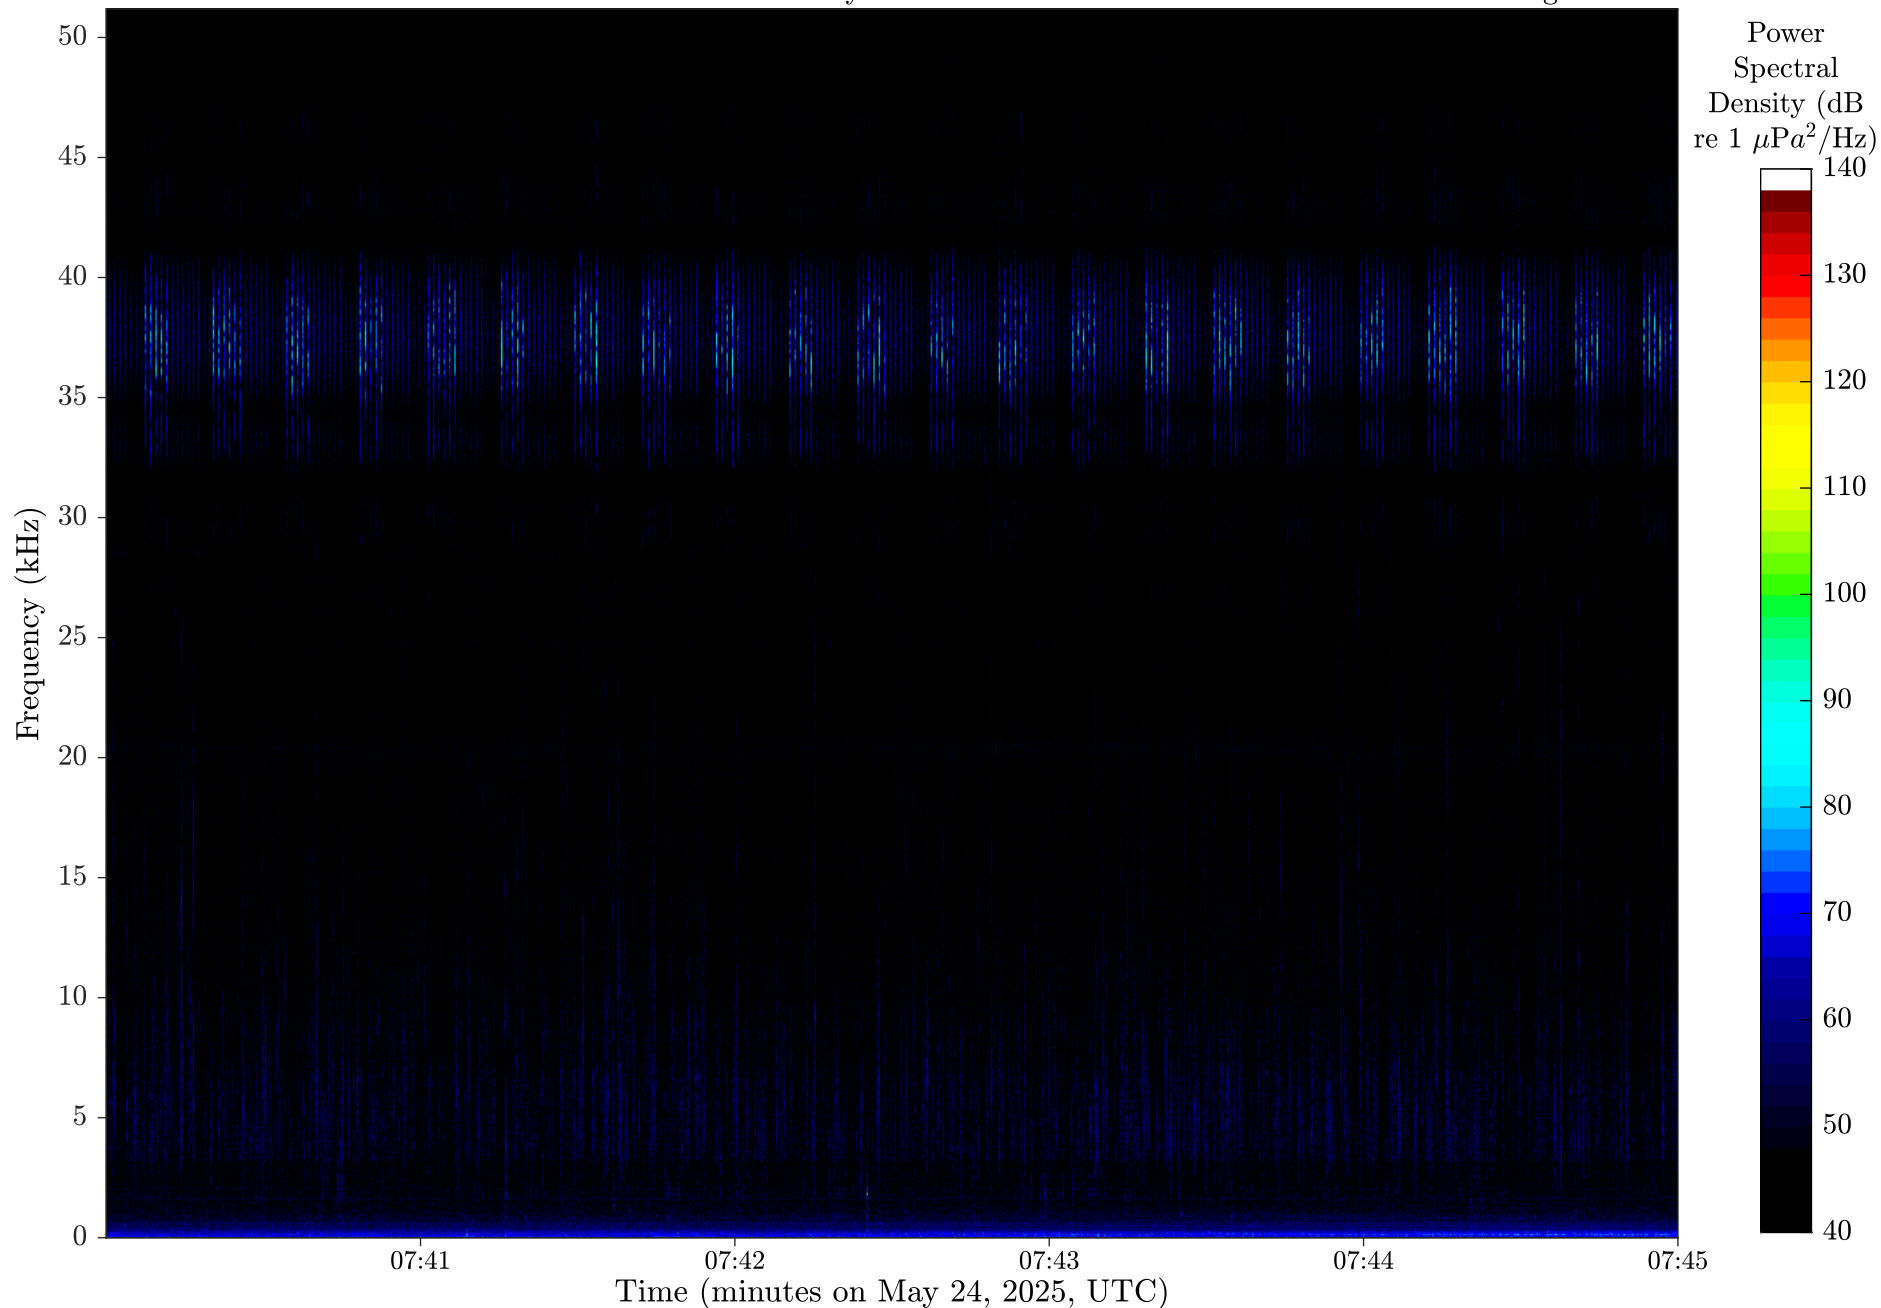


Comments: 36.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:31:53 UTC

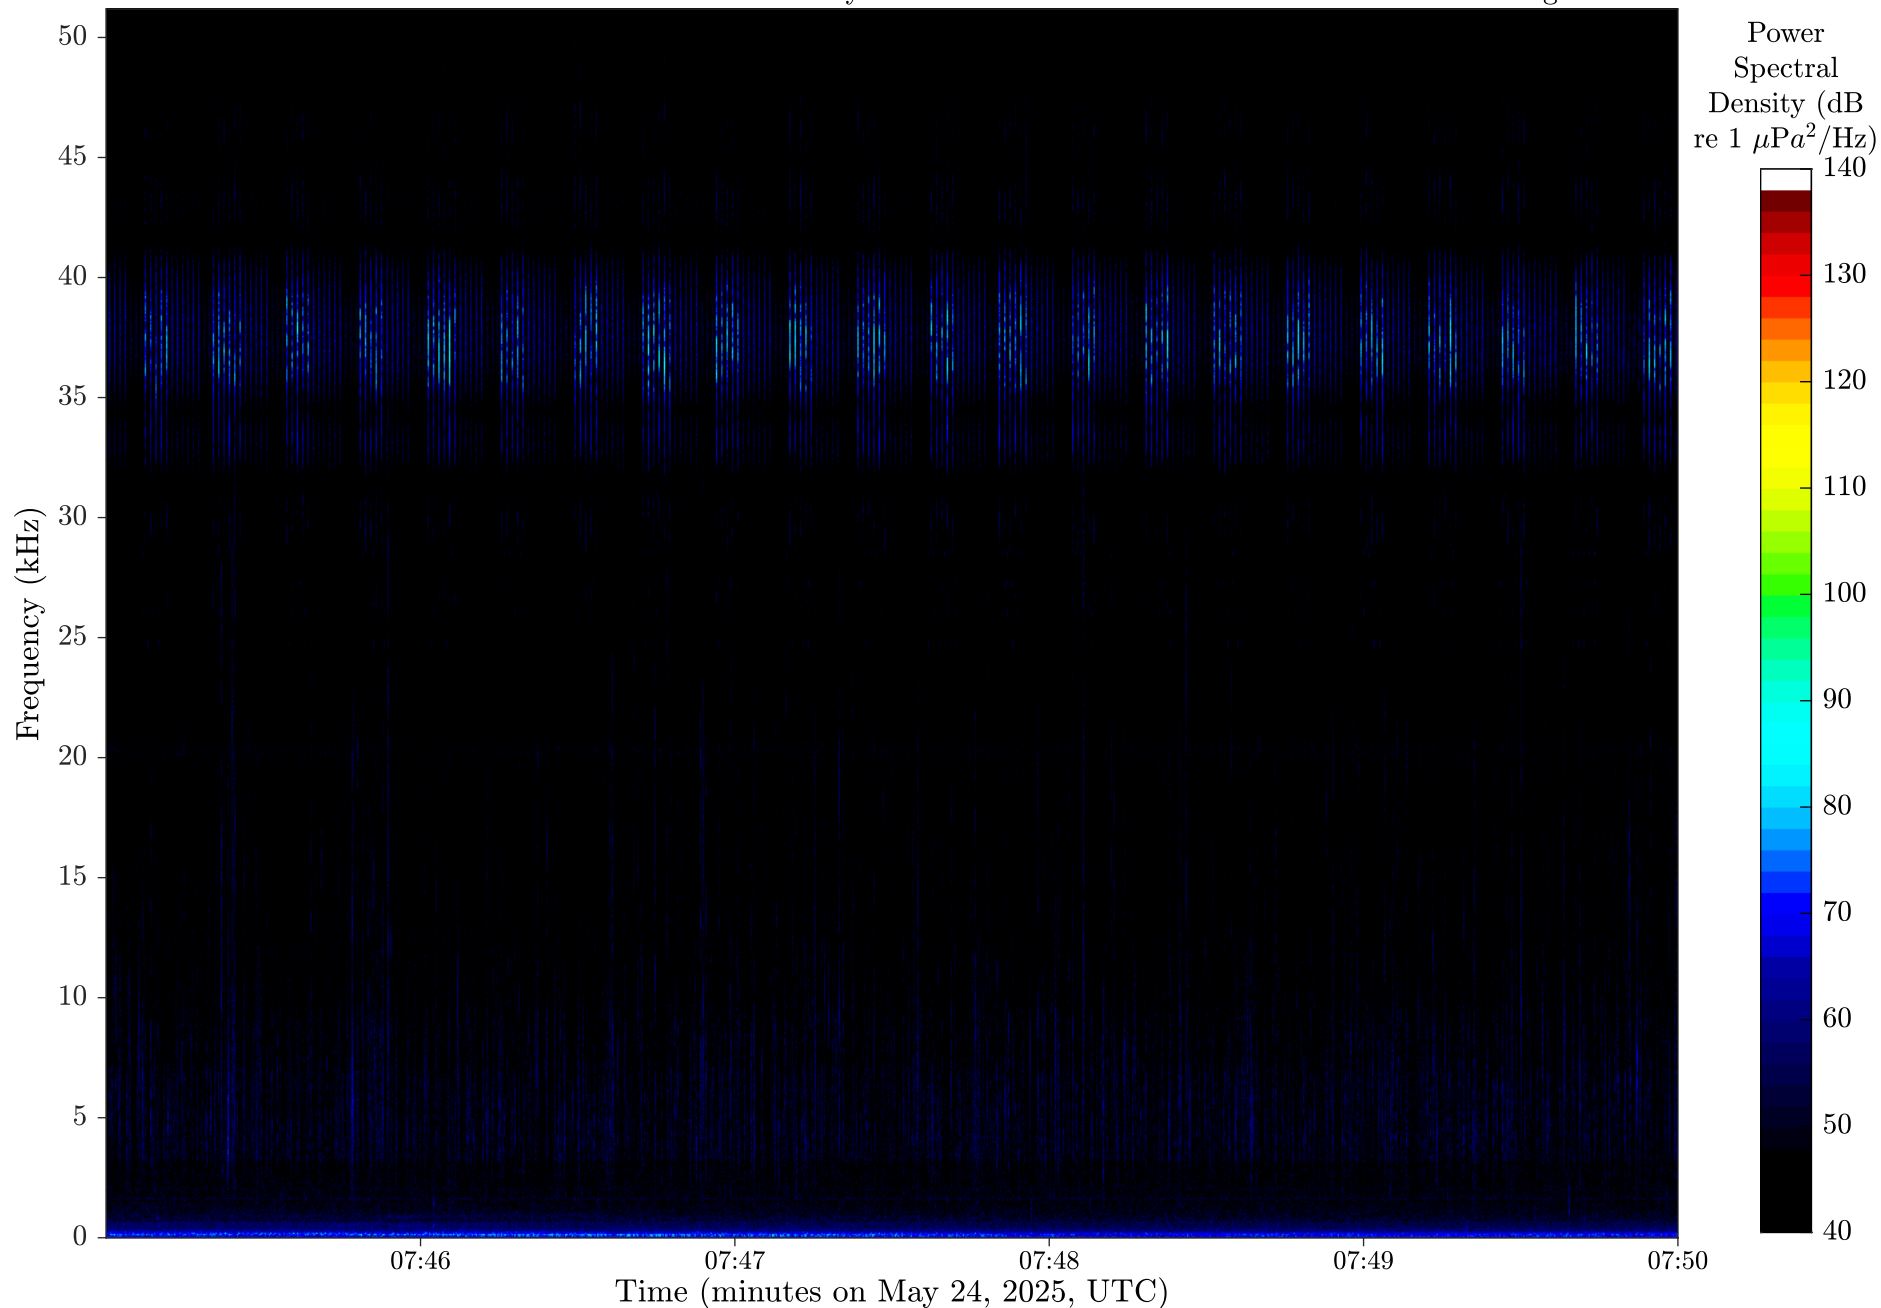


Comments: 36.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:32:02 UTC

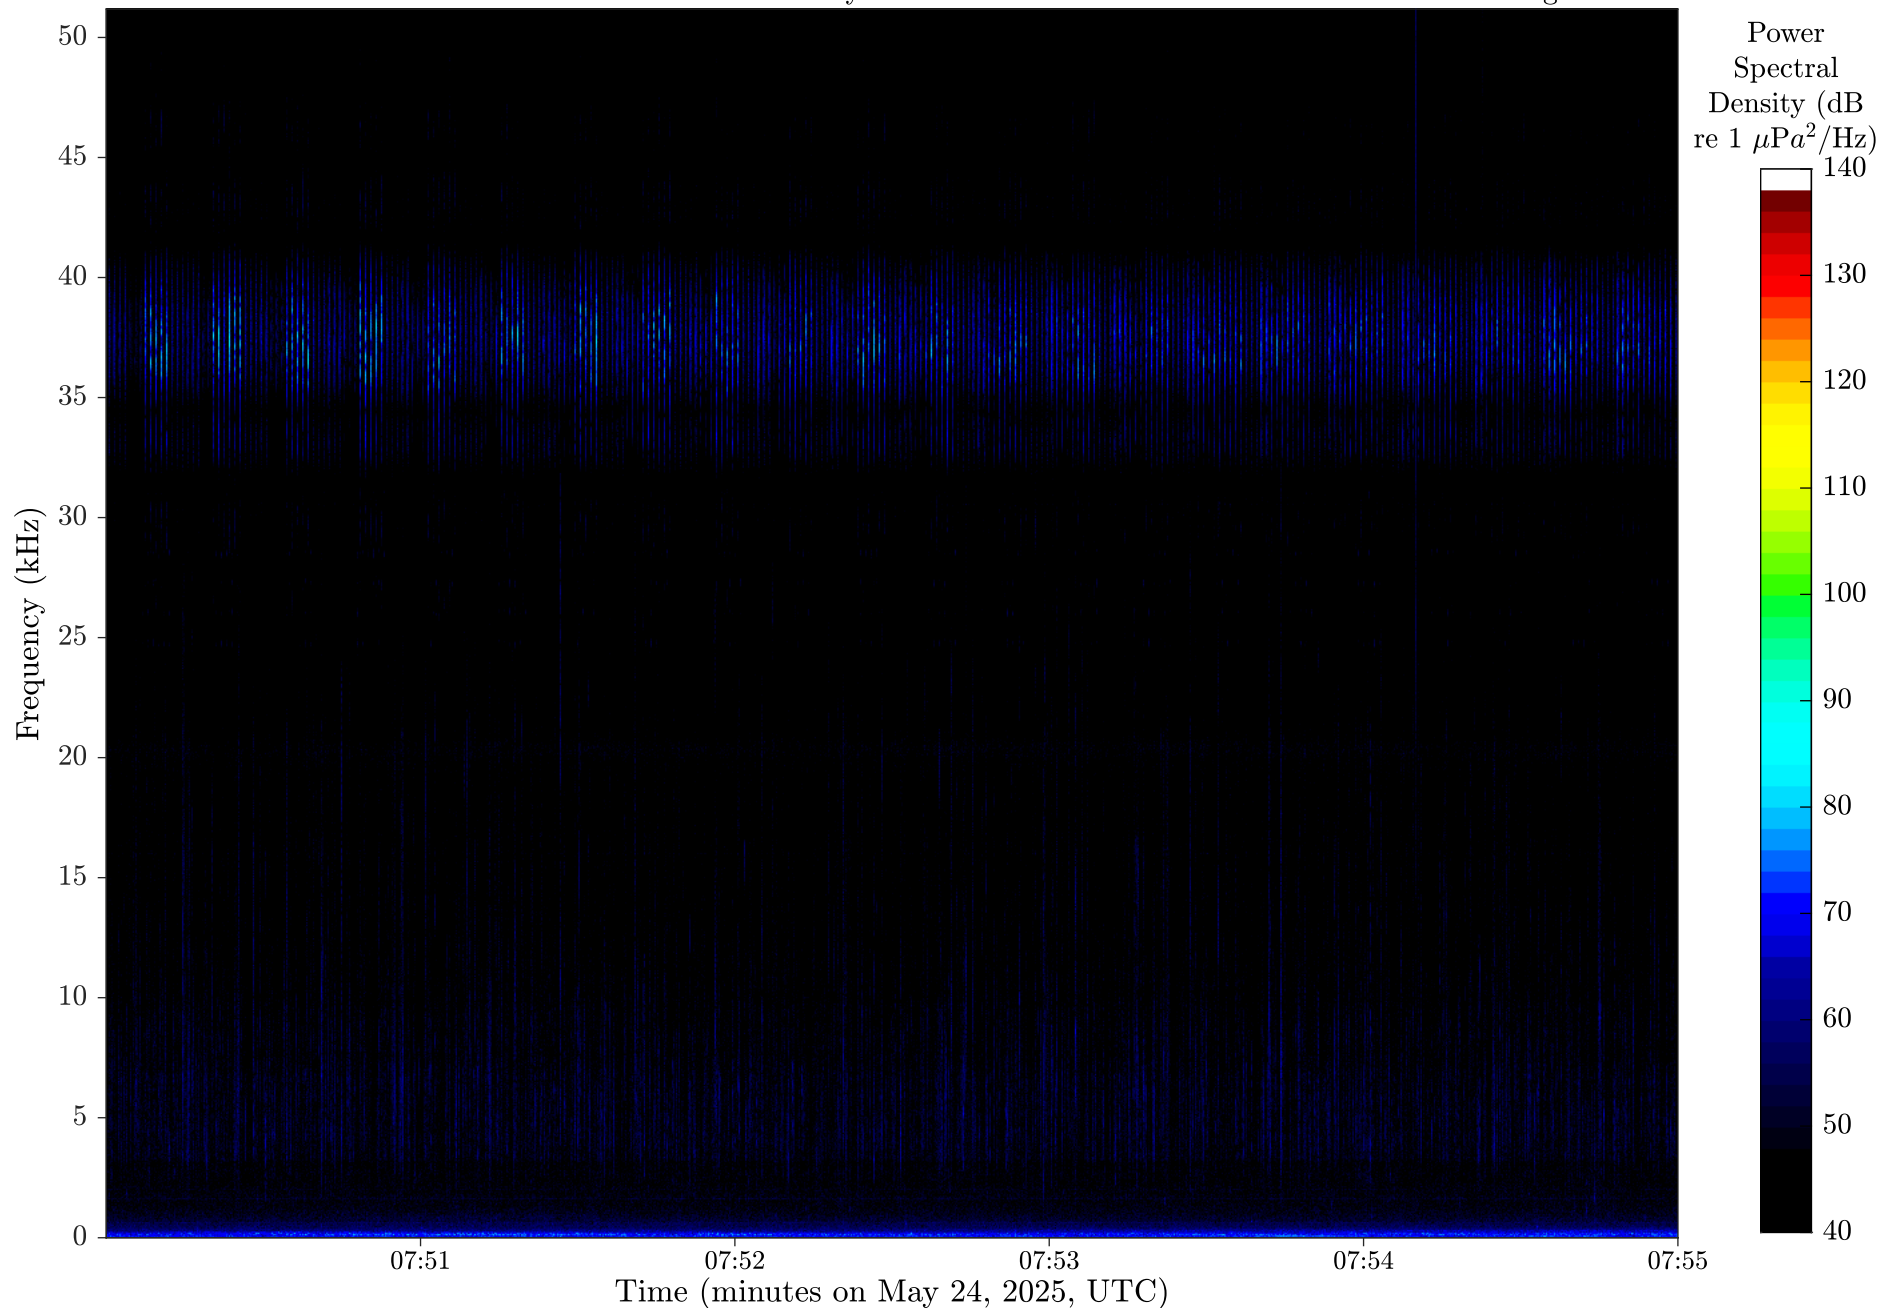


Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:32:11 UTC

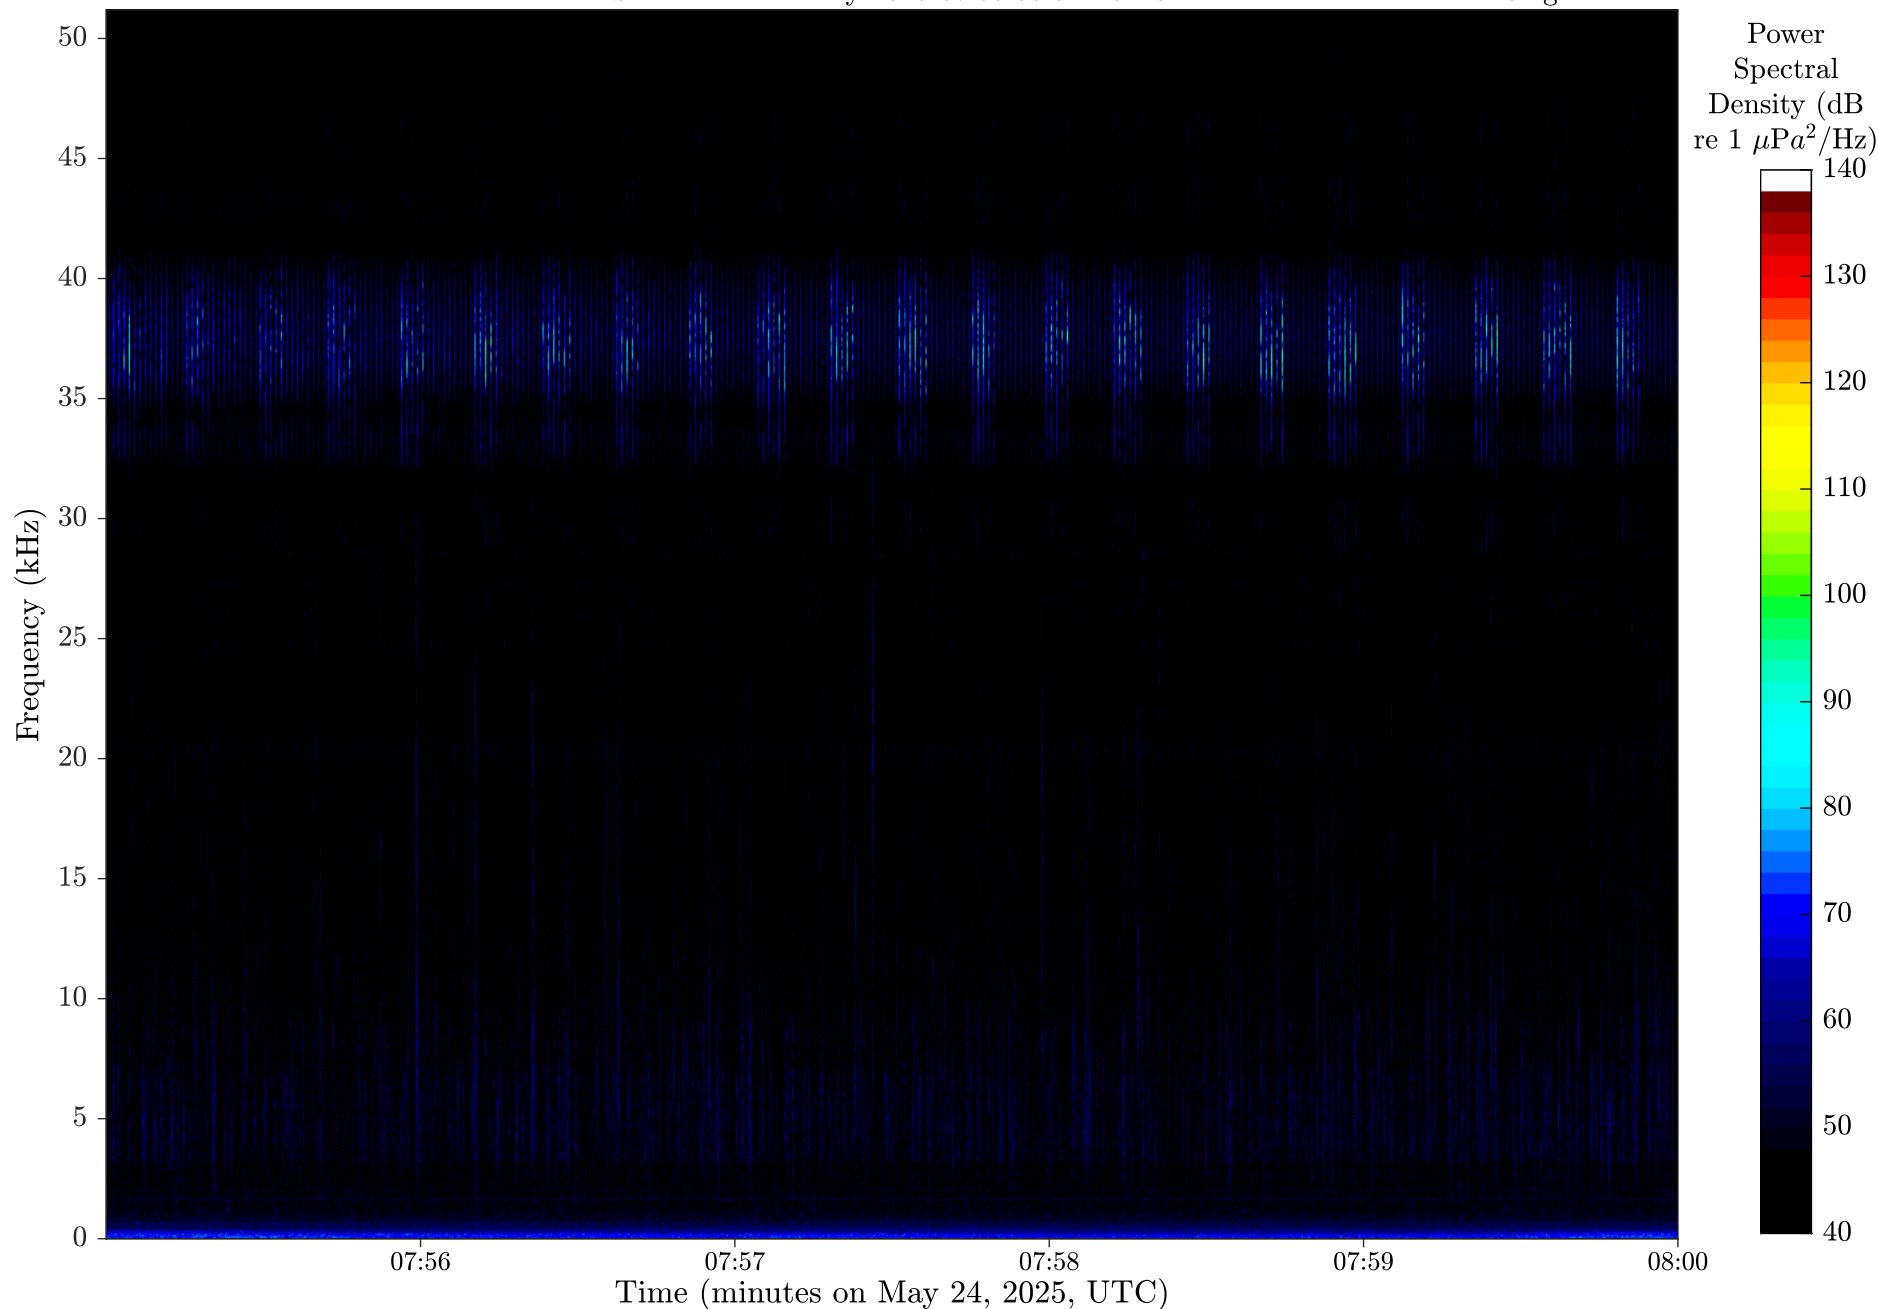

Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:32:20 UTC

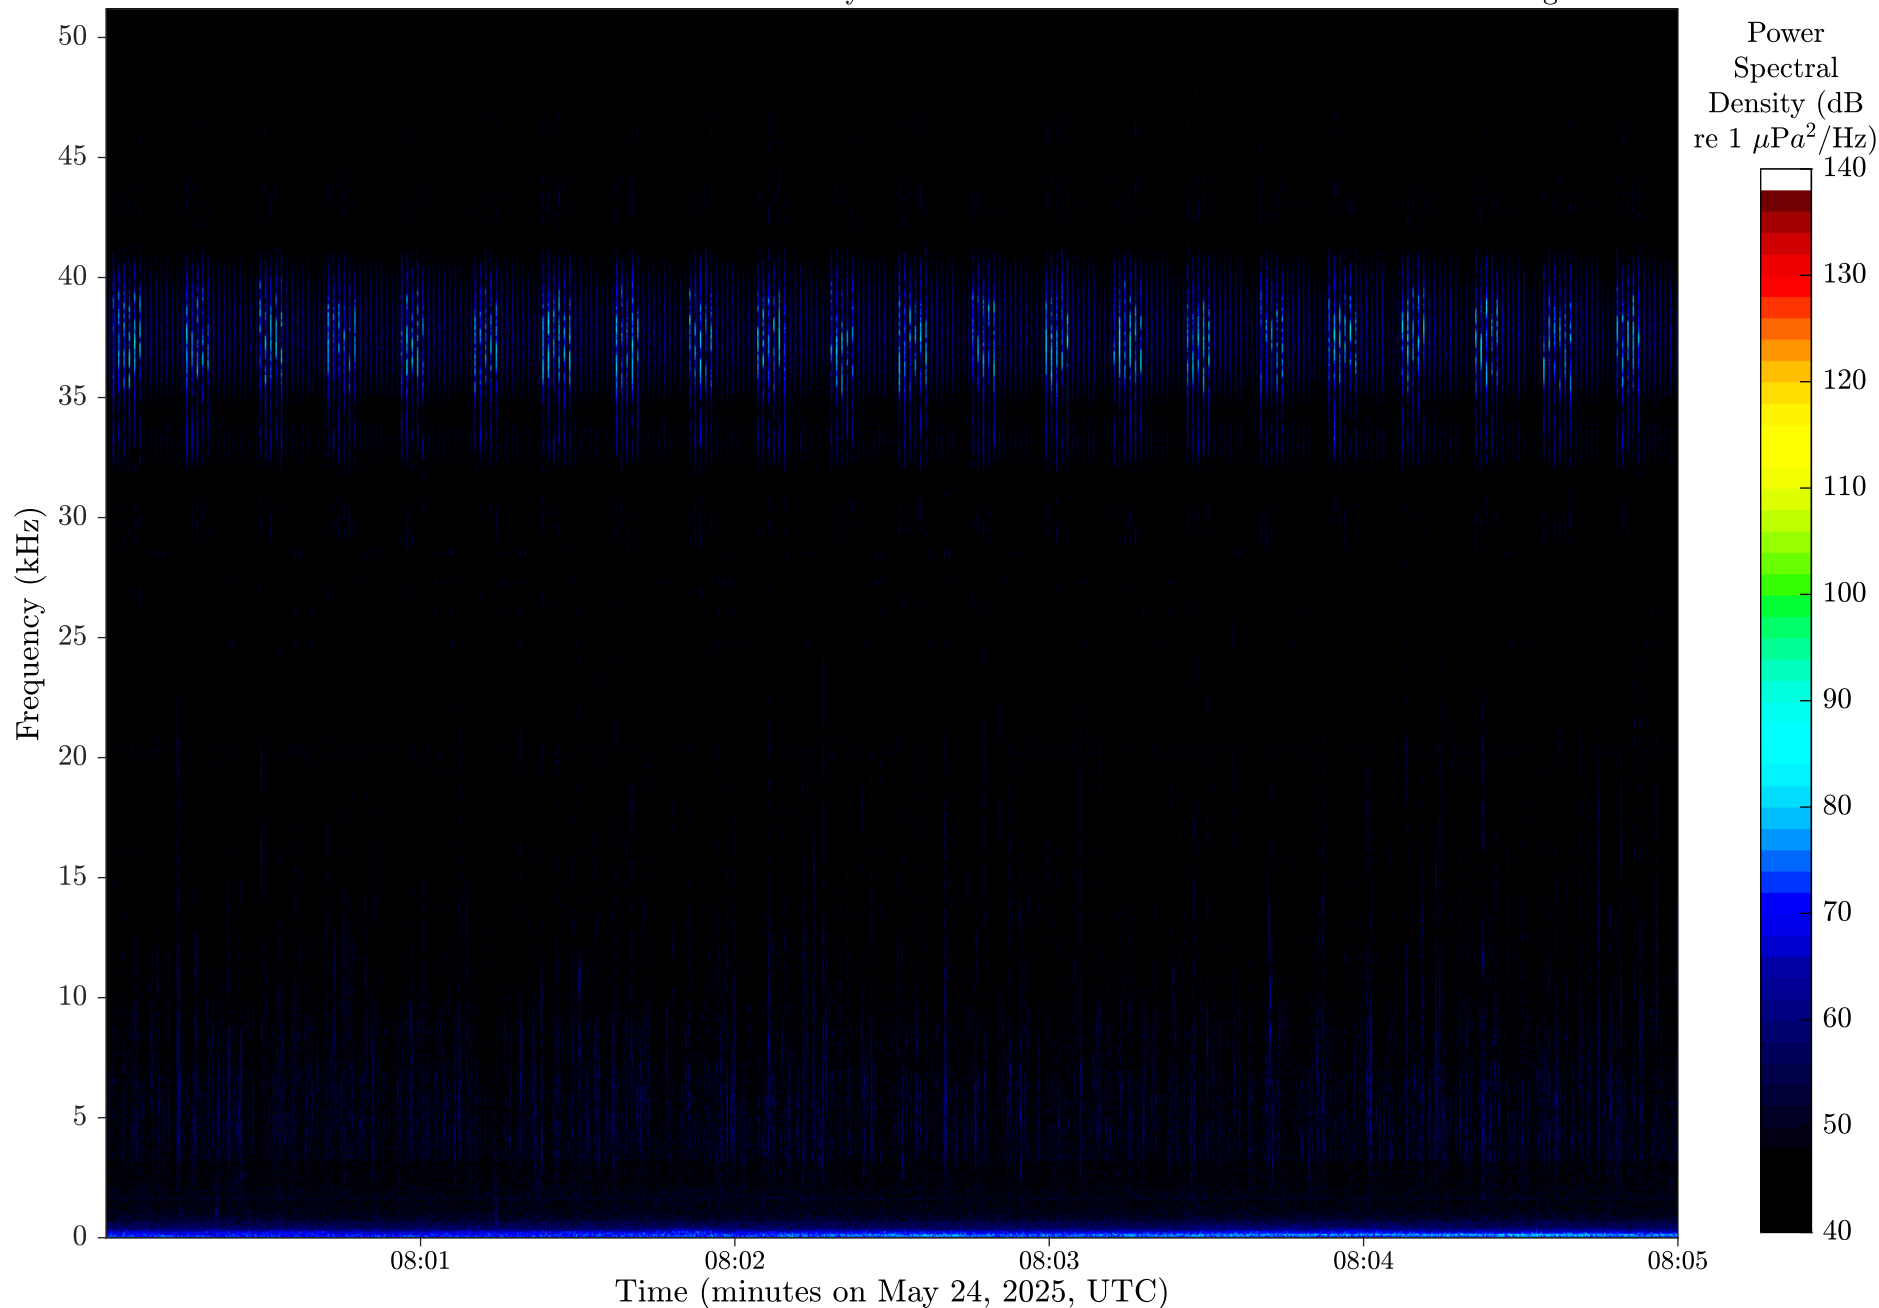

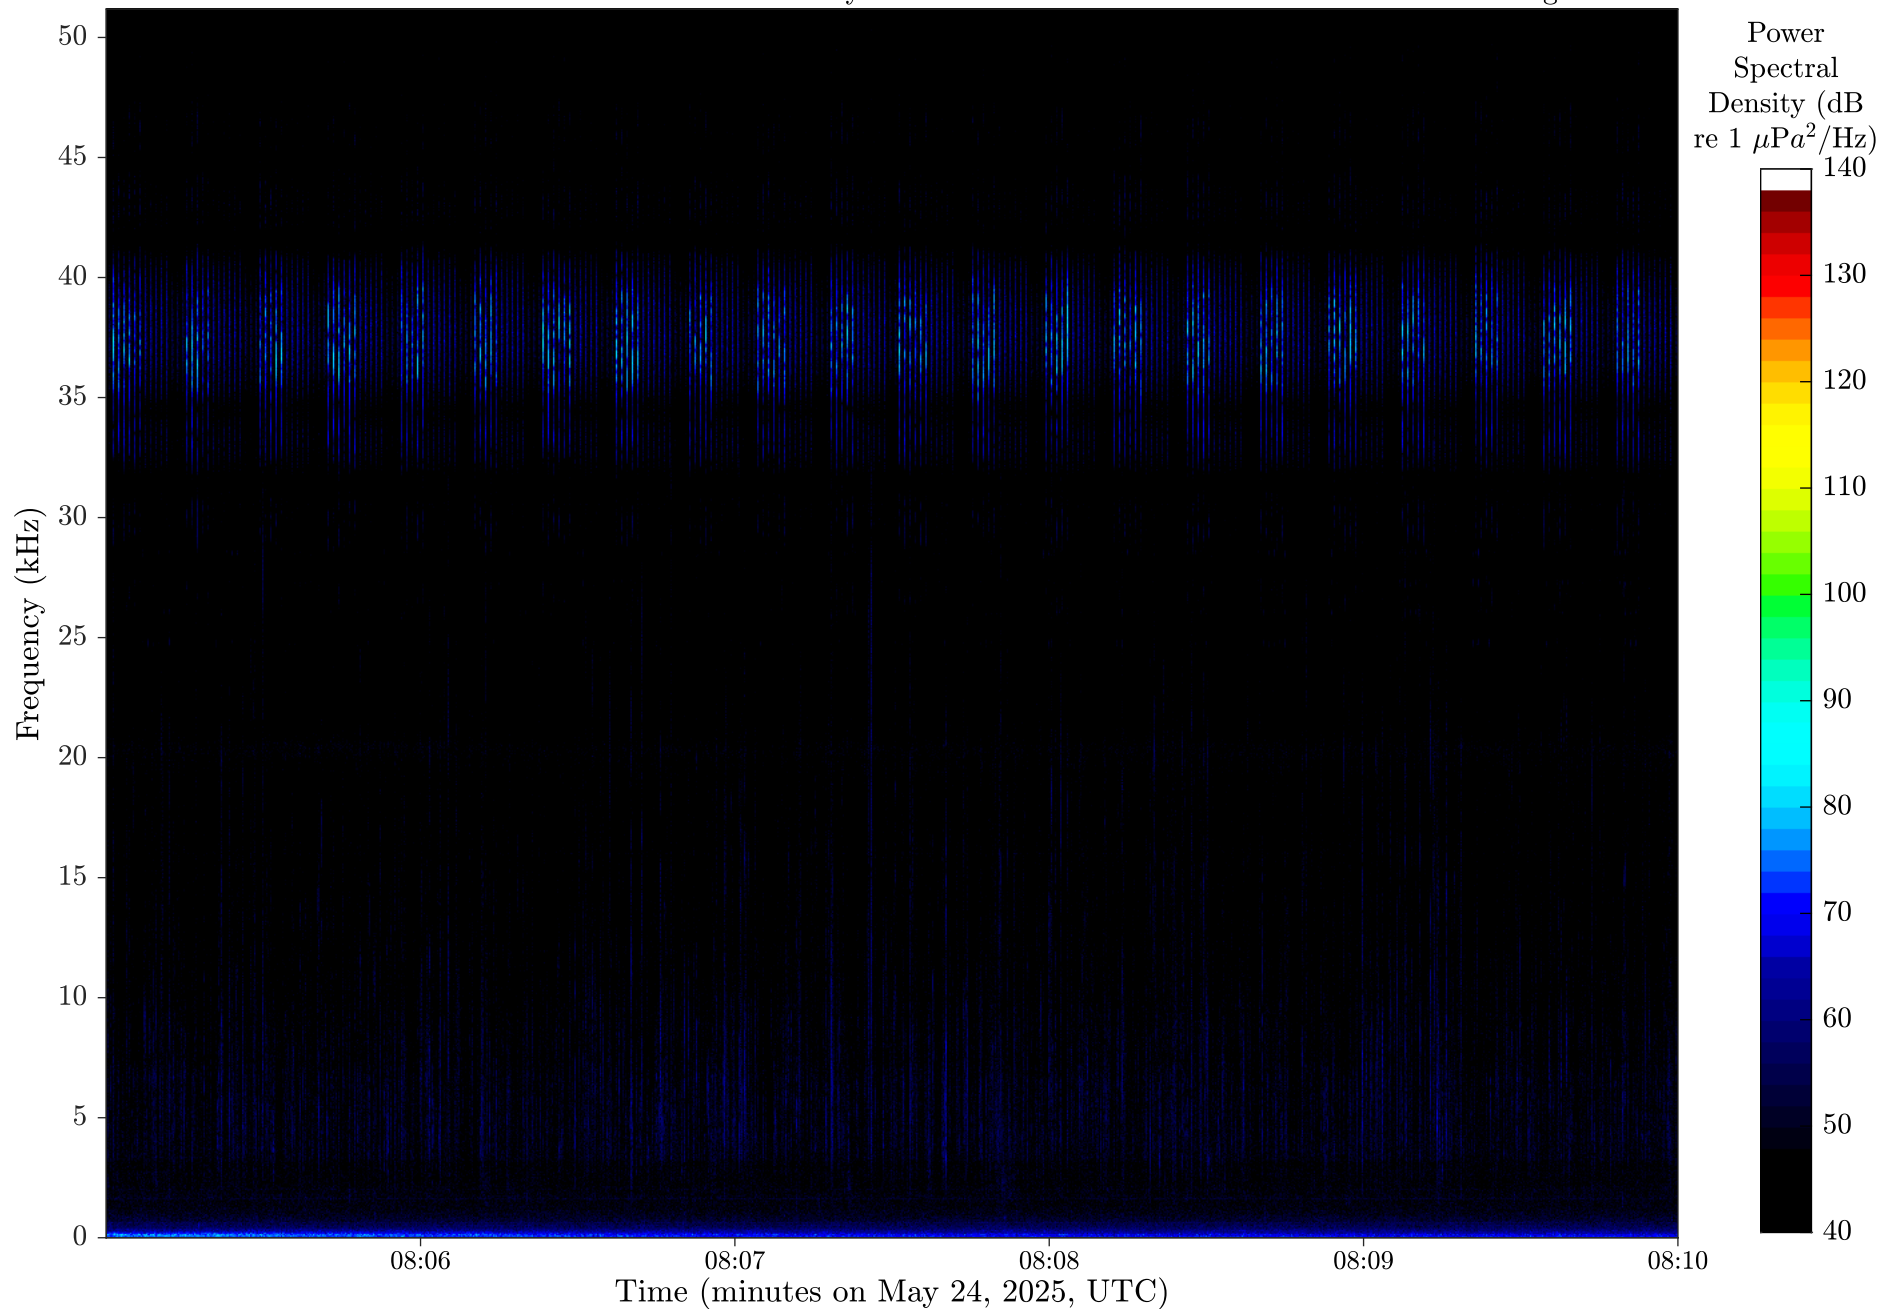


Comments: 36.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:32:36 UTC

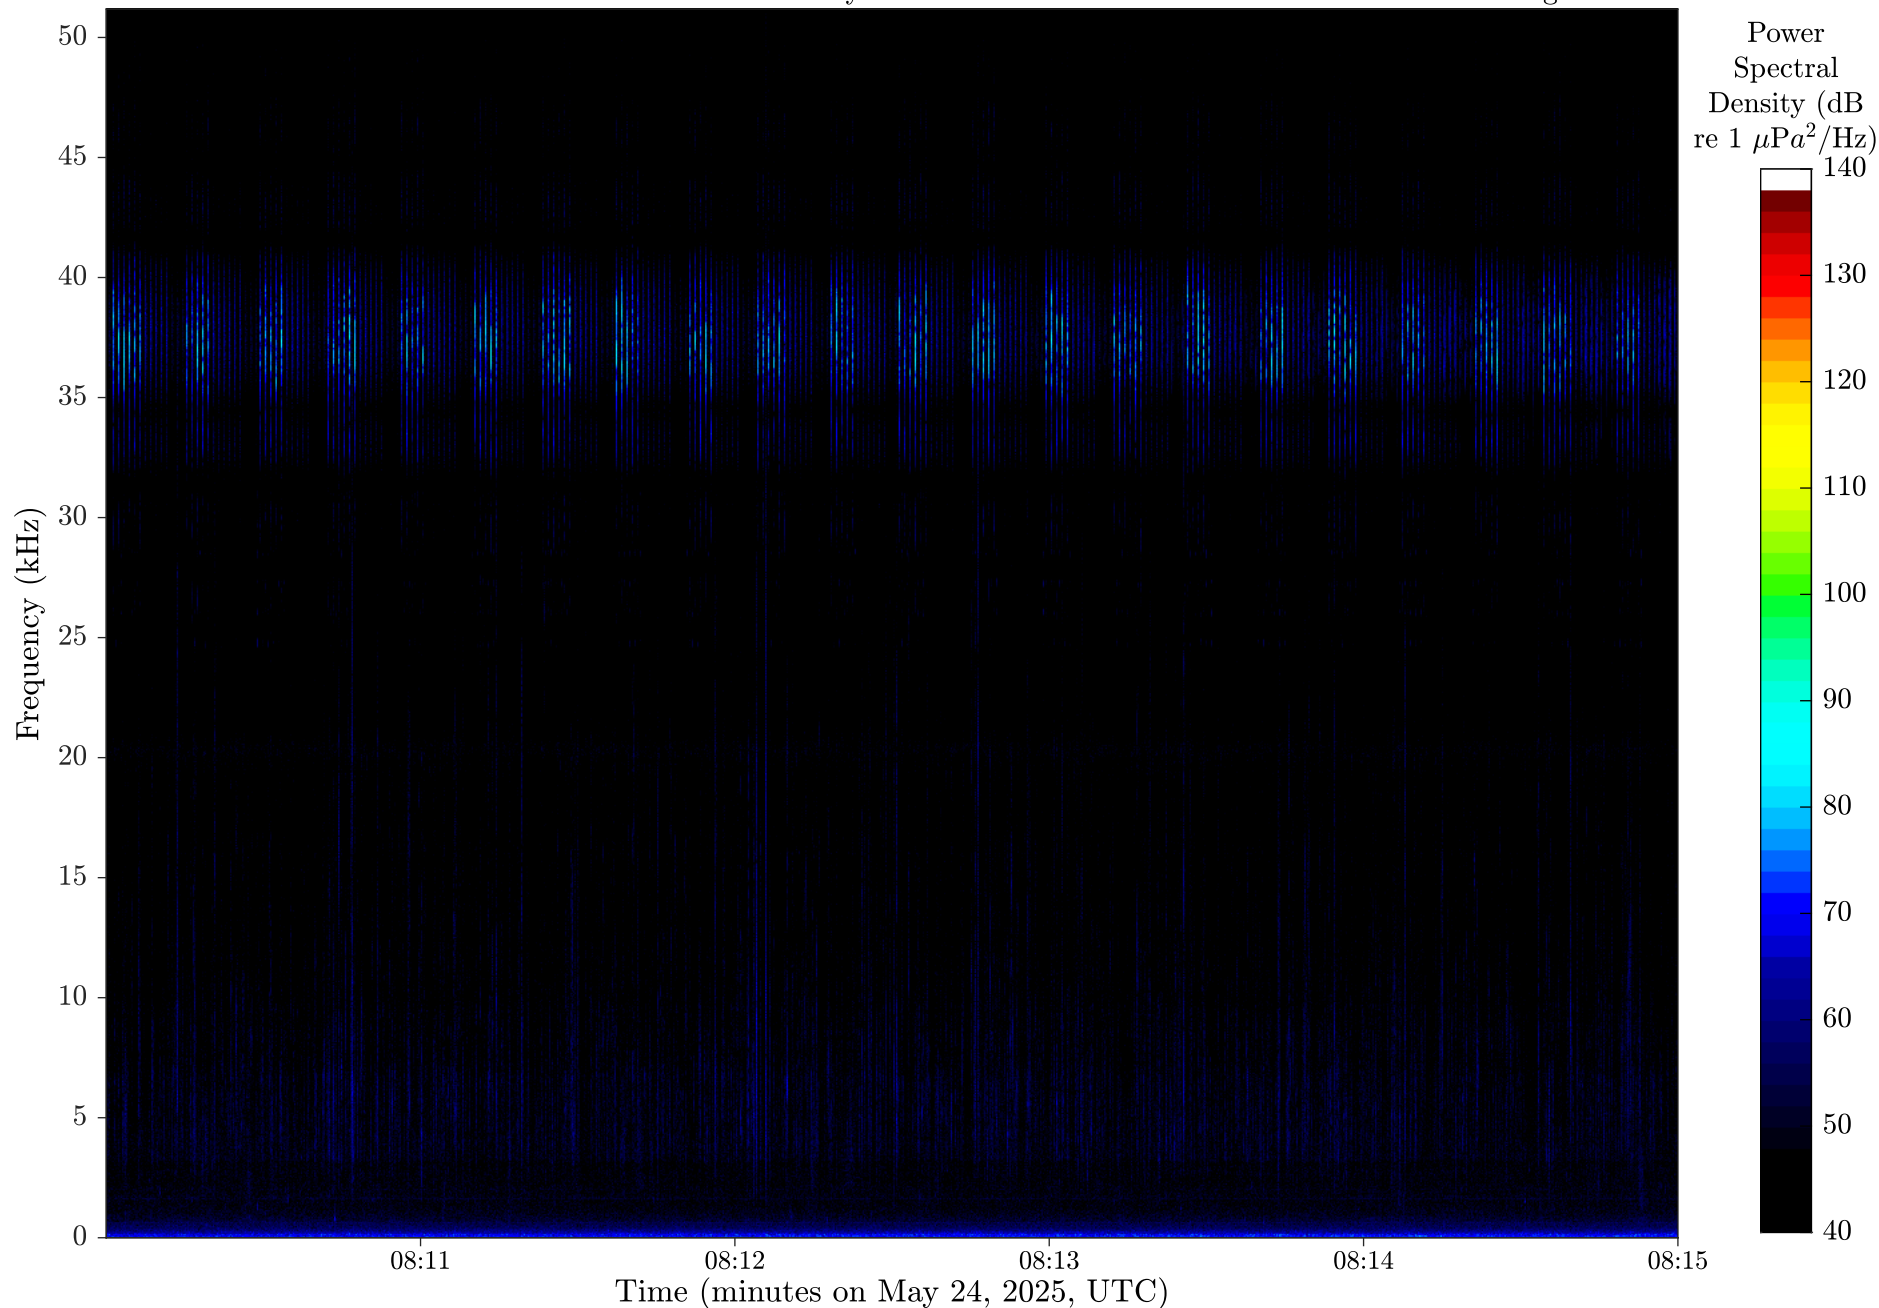

Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:32:45 UTC

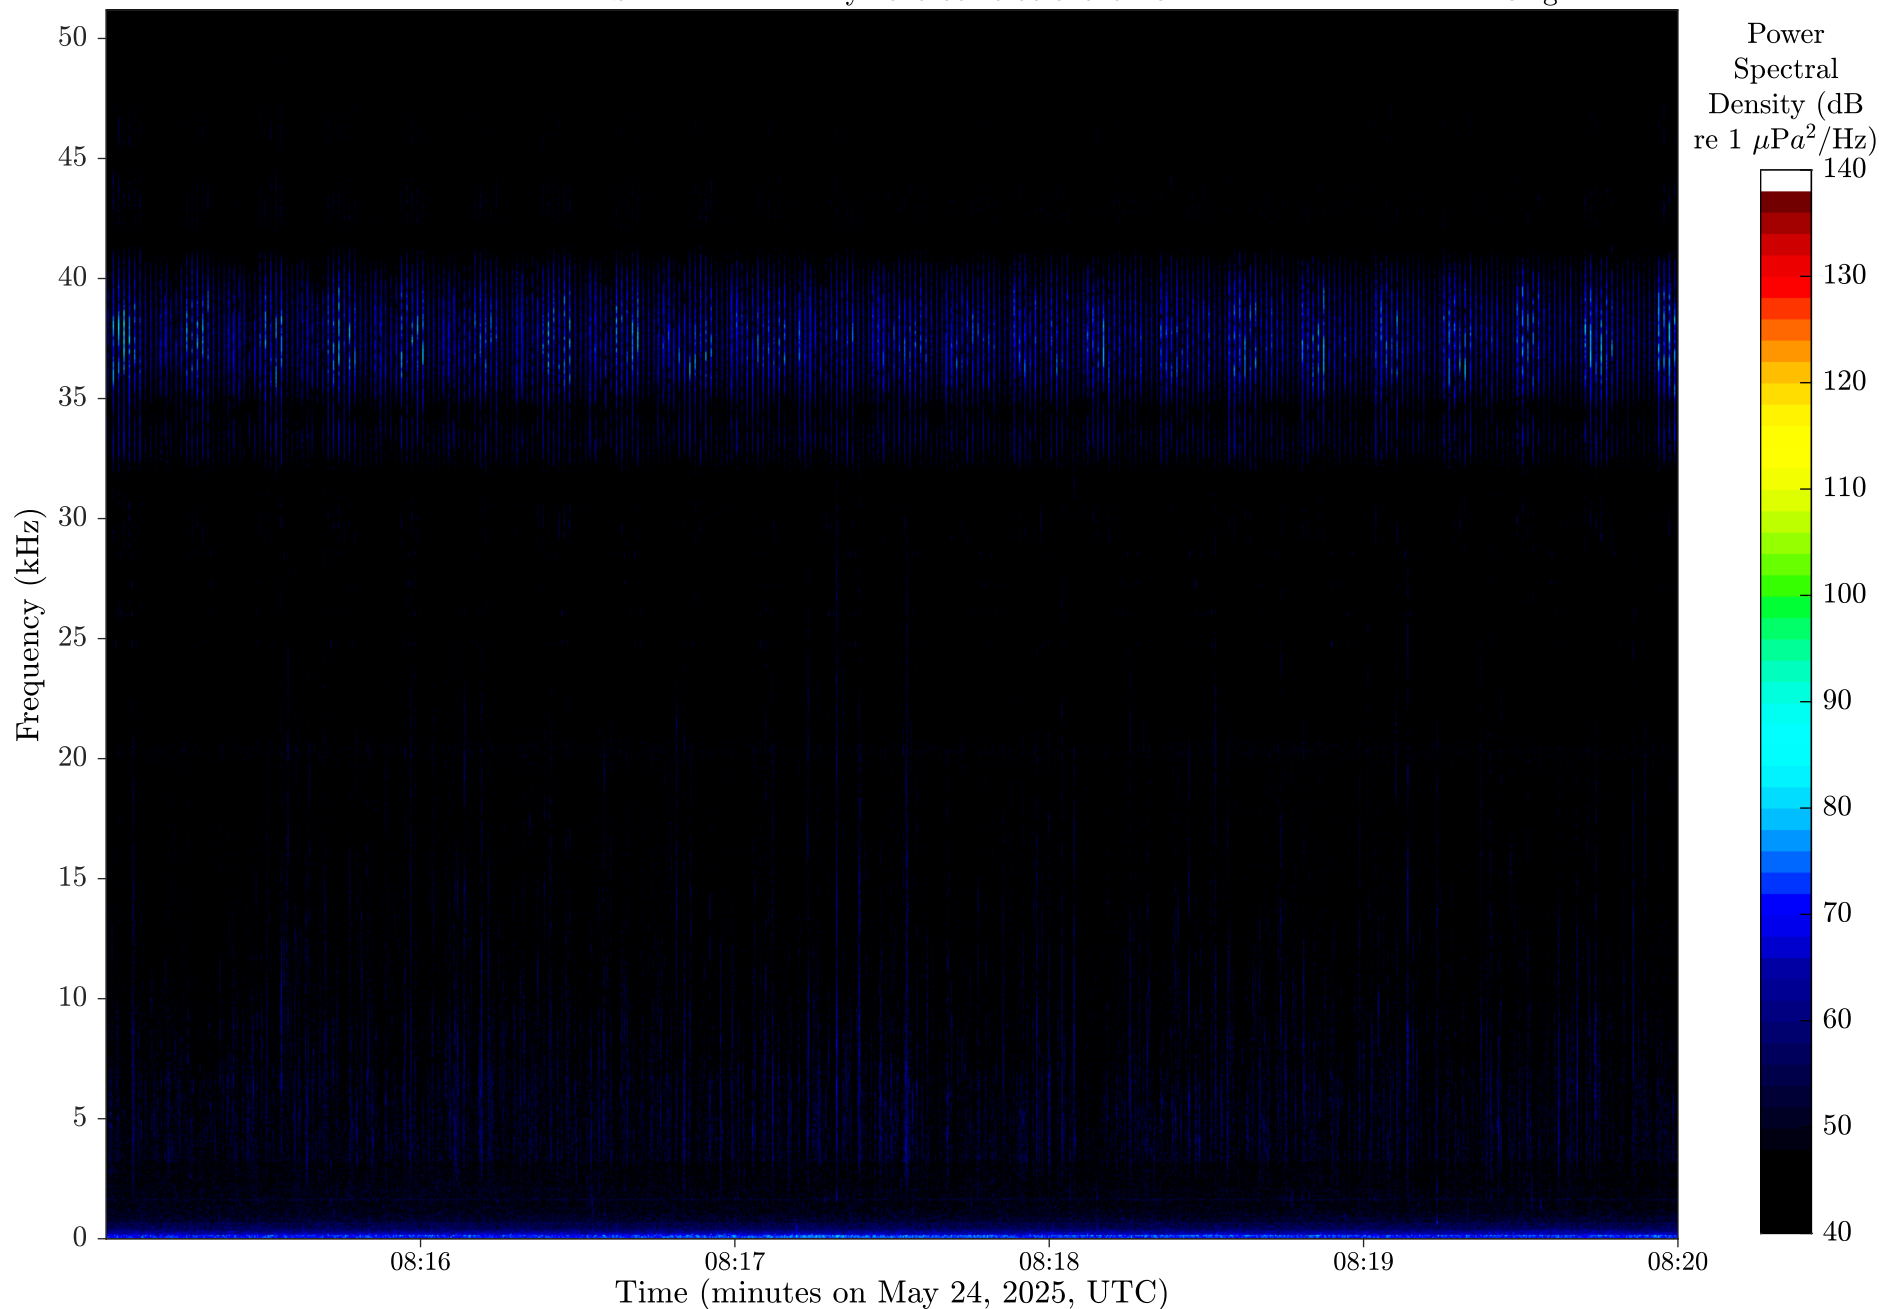

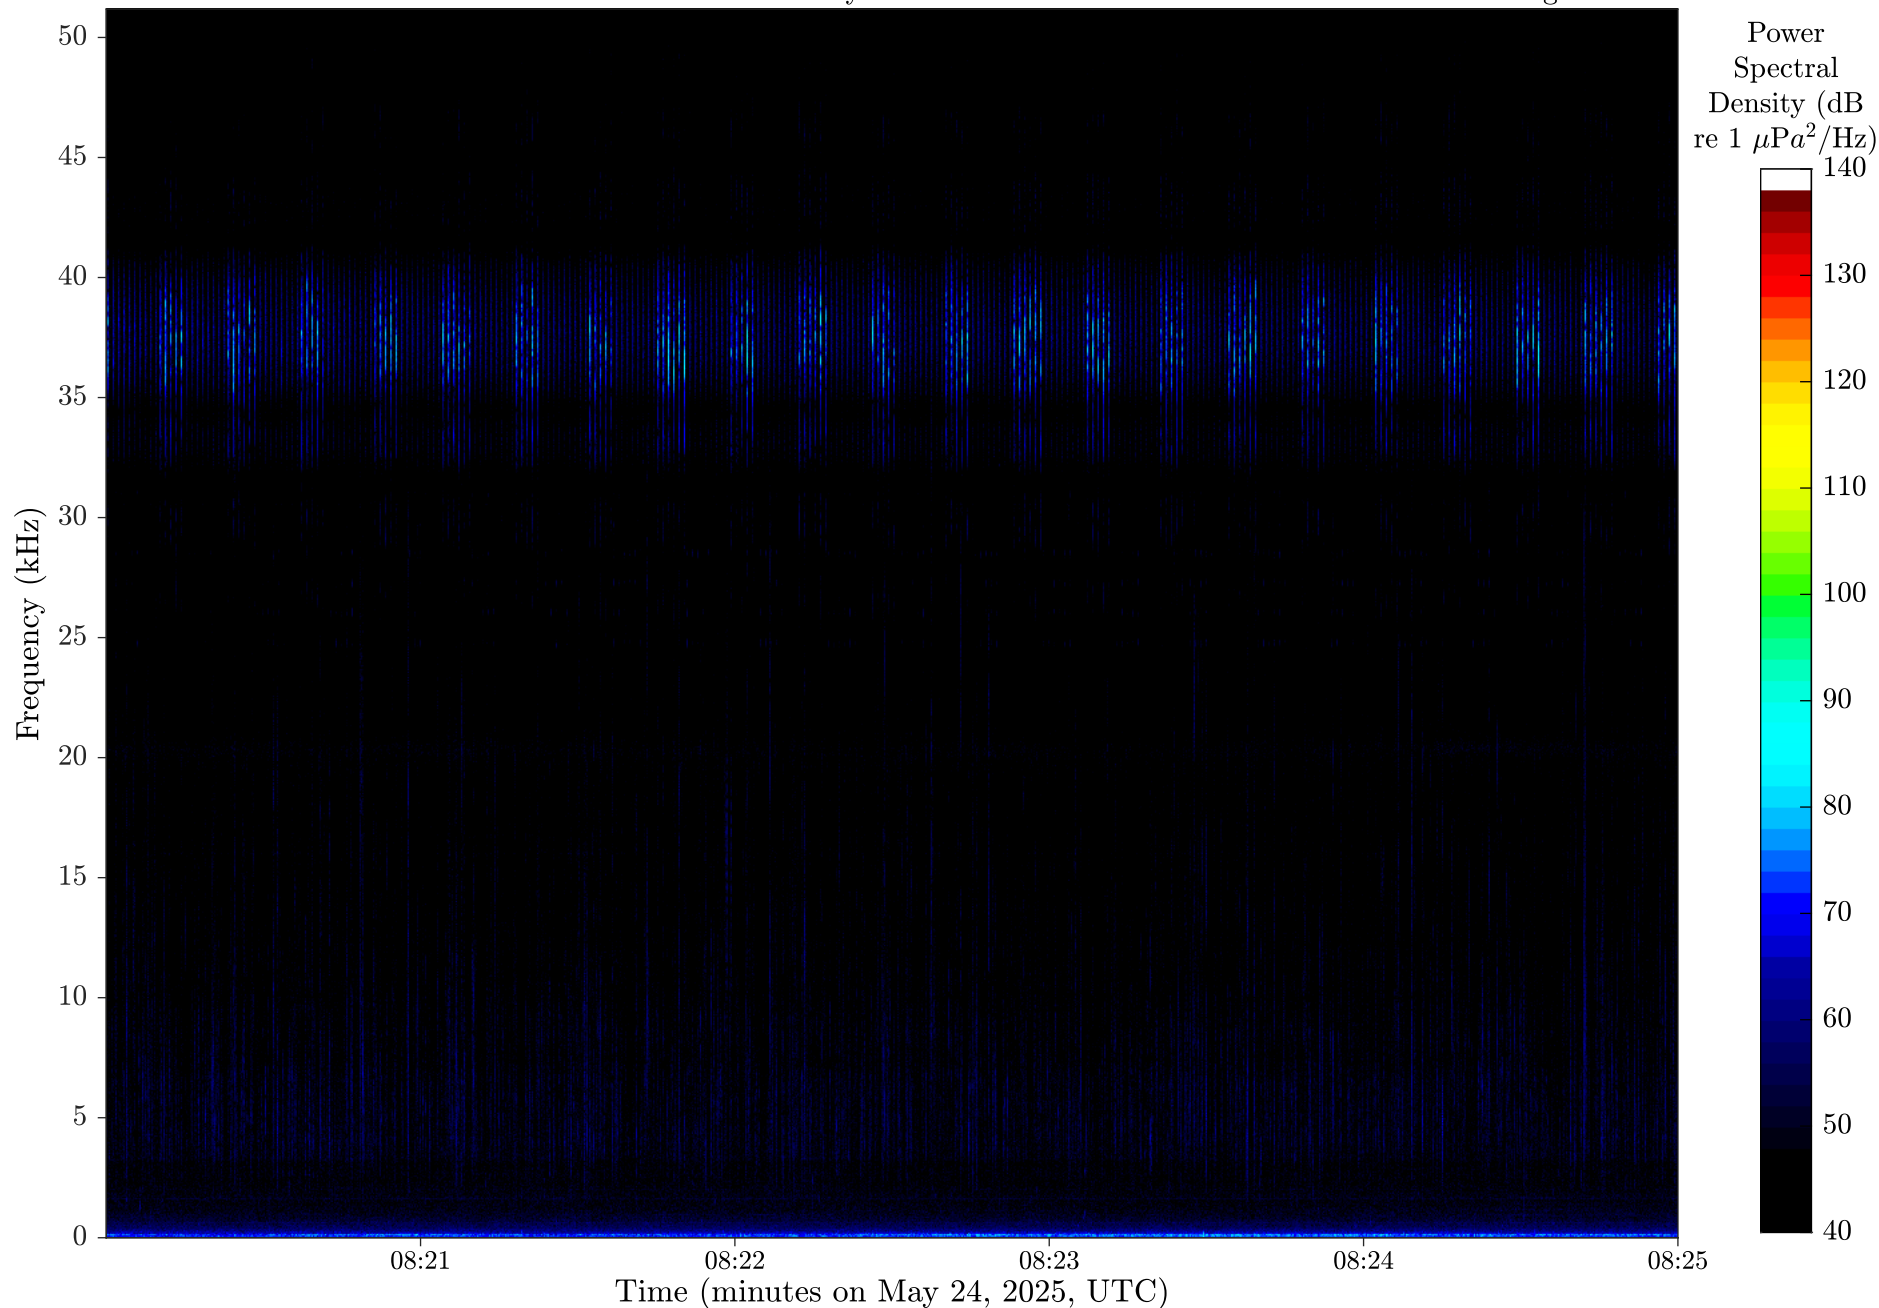


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:33:02 UTC

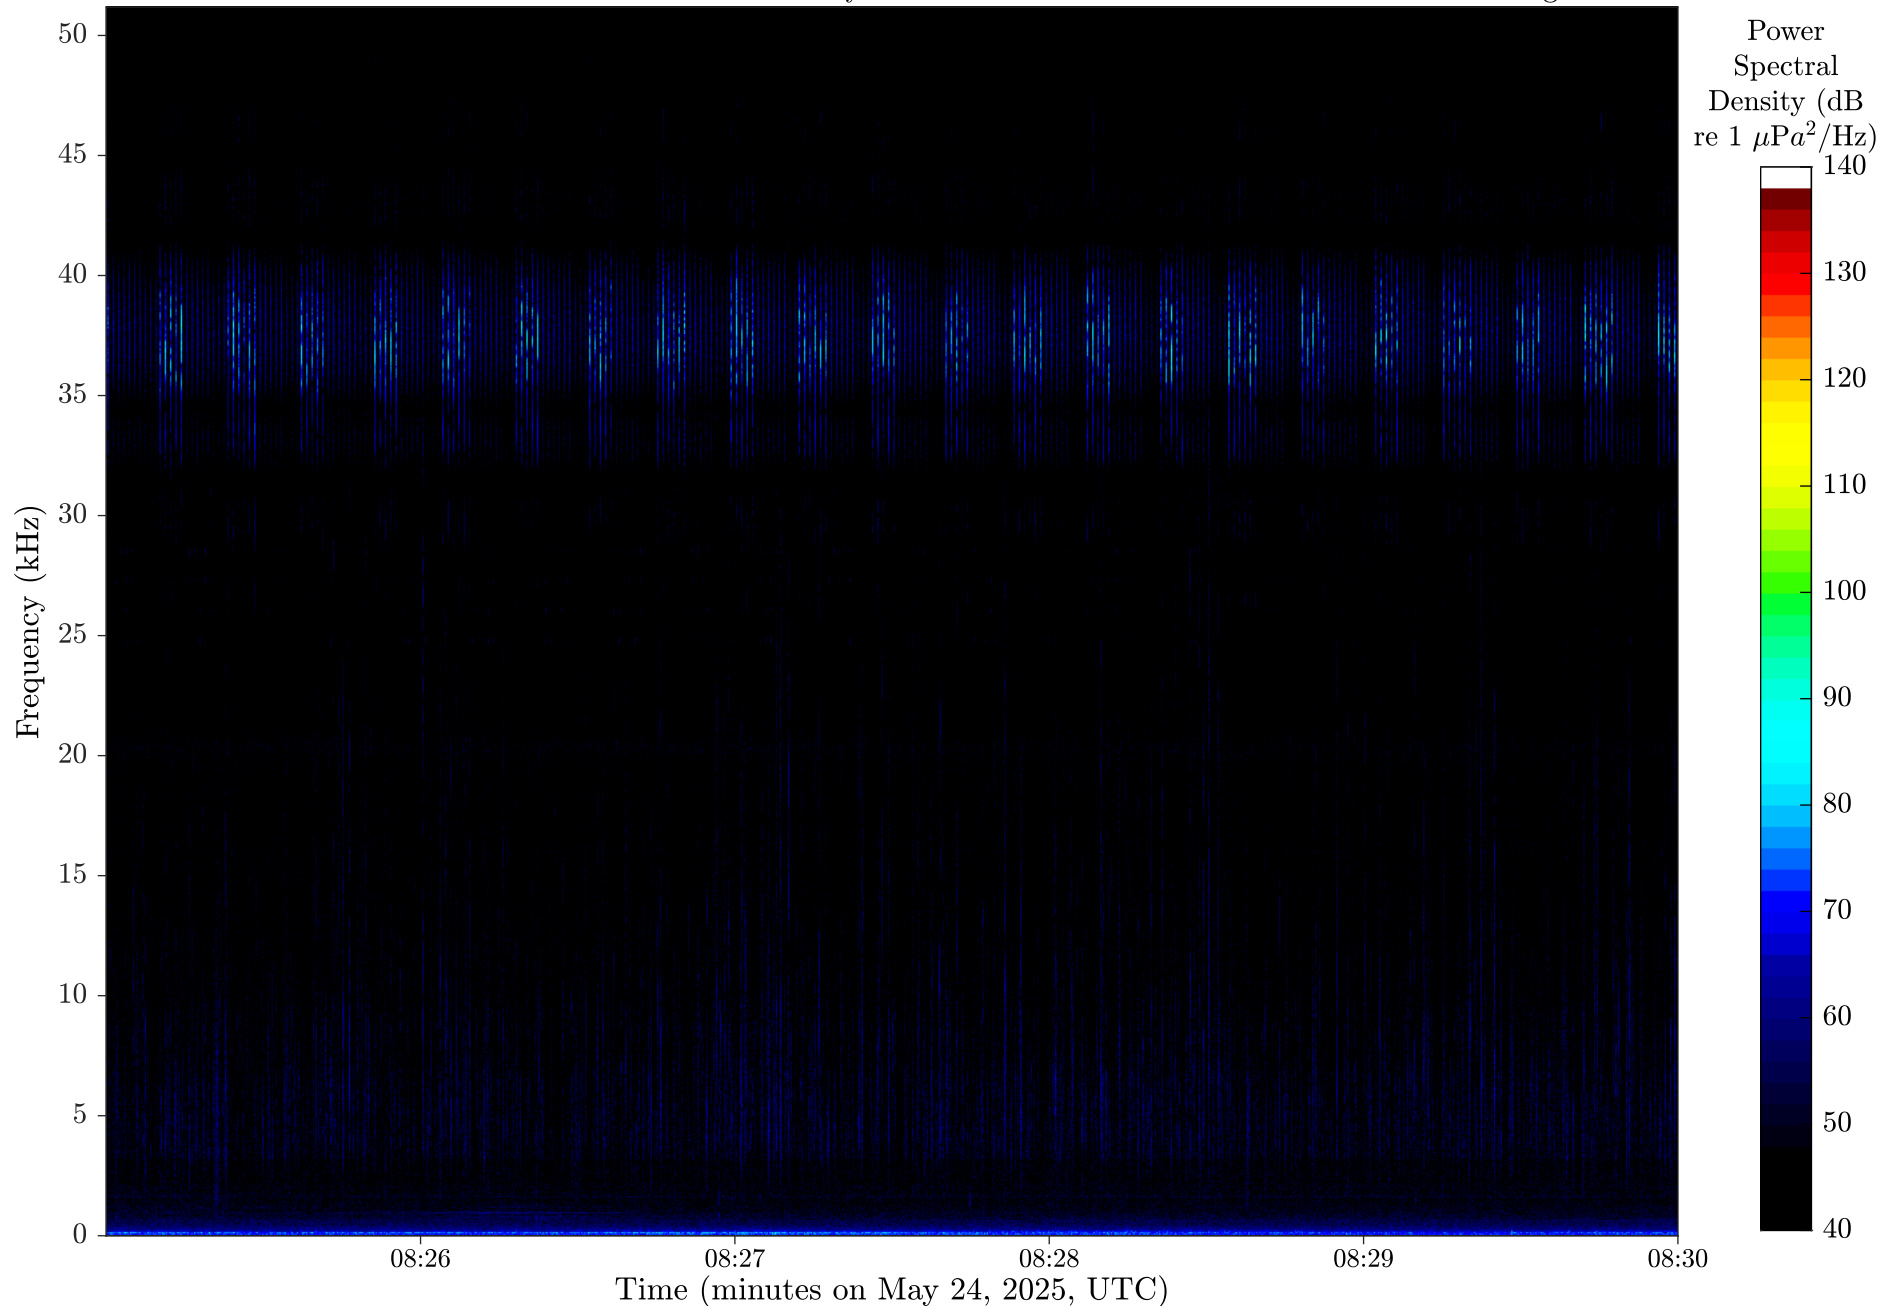

Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:33:10 UTC

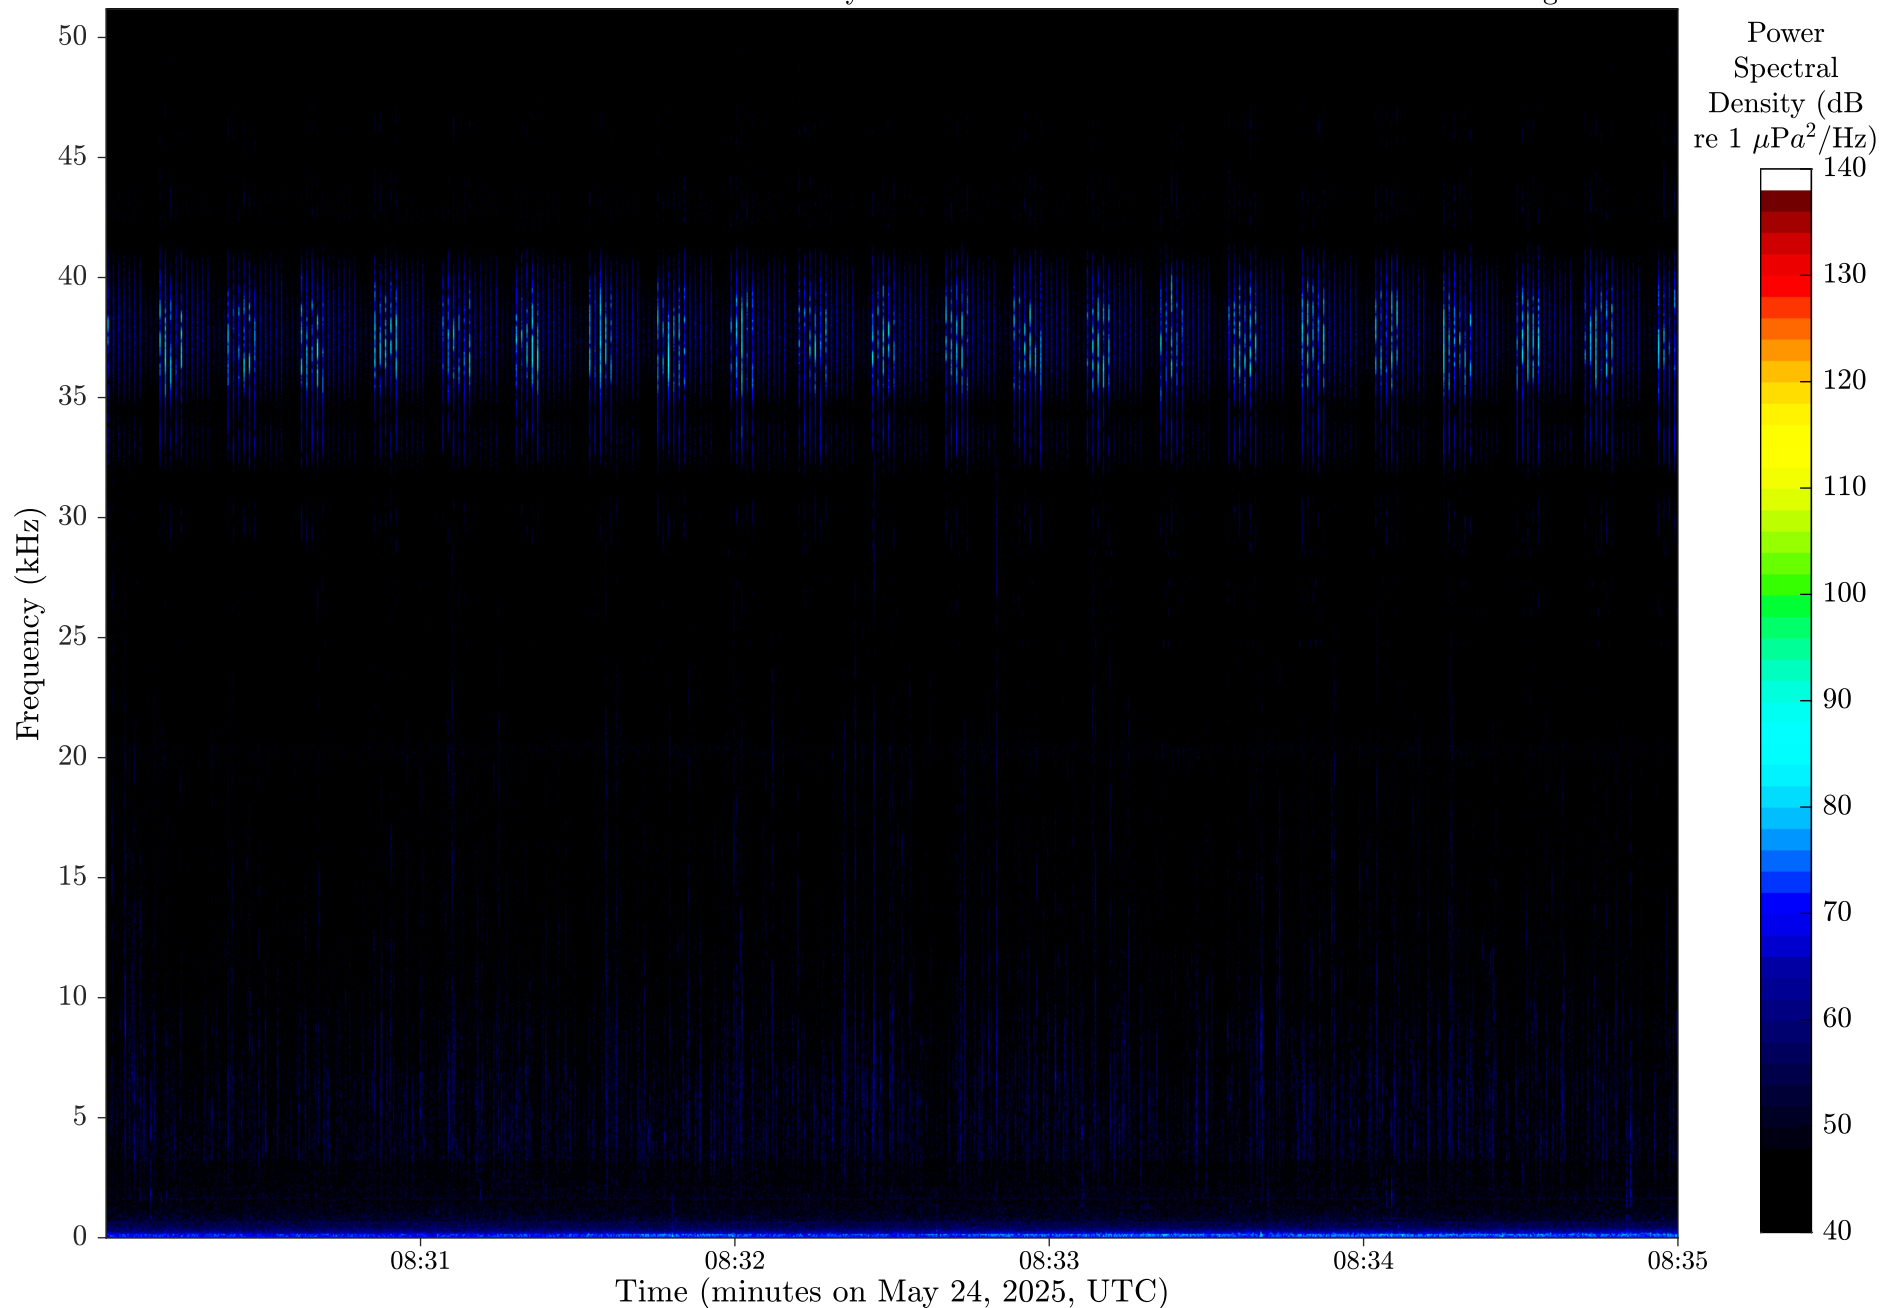


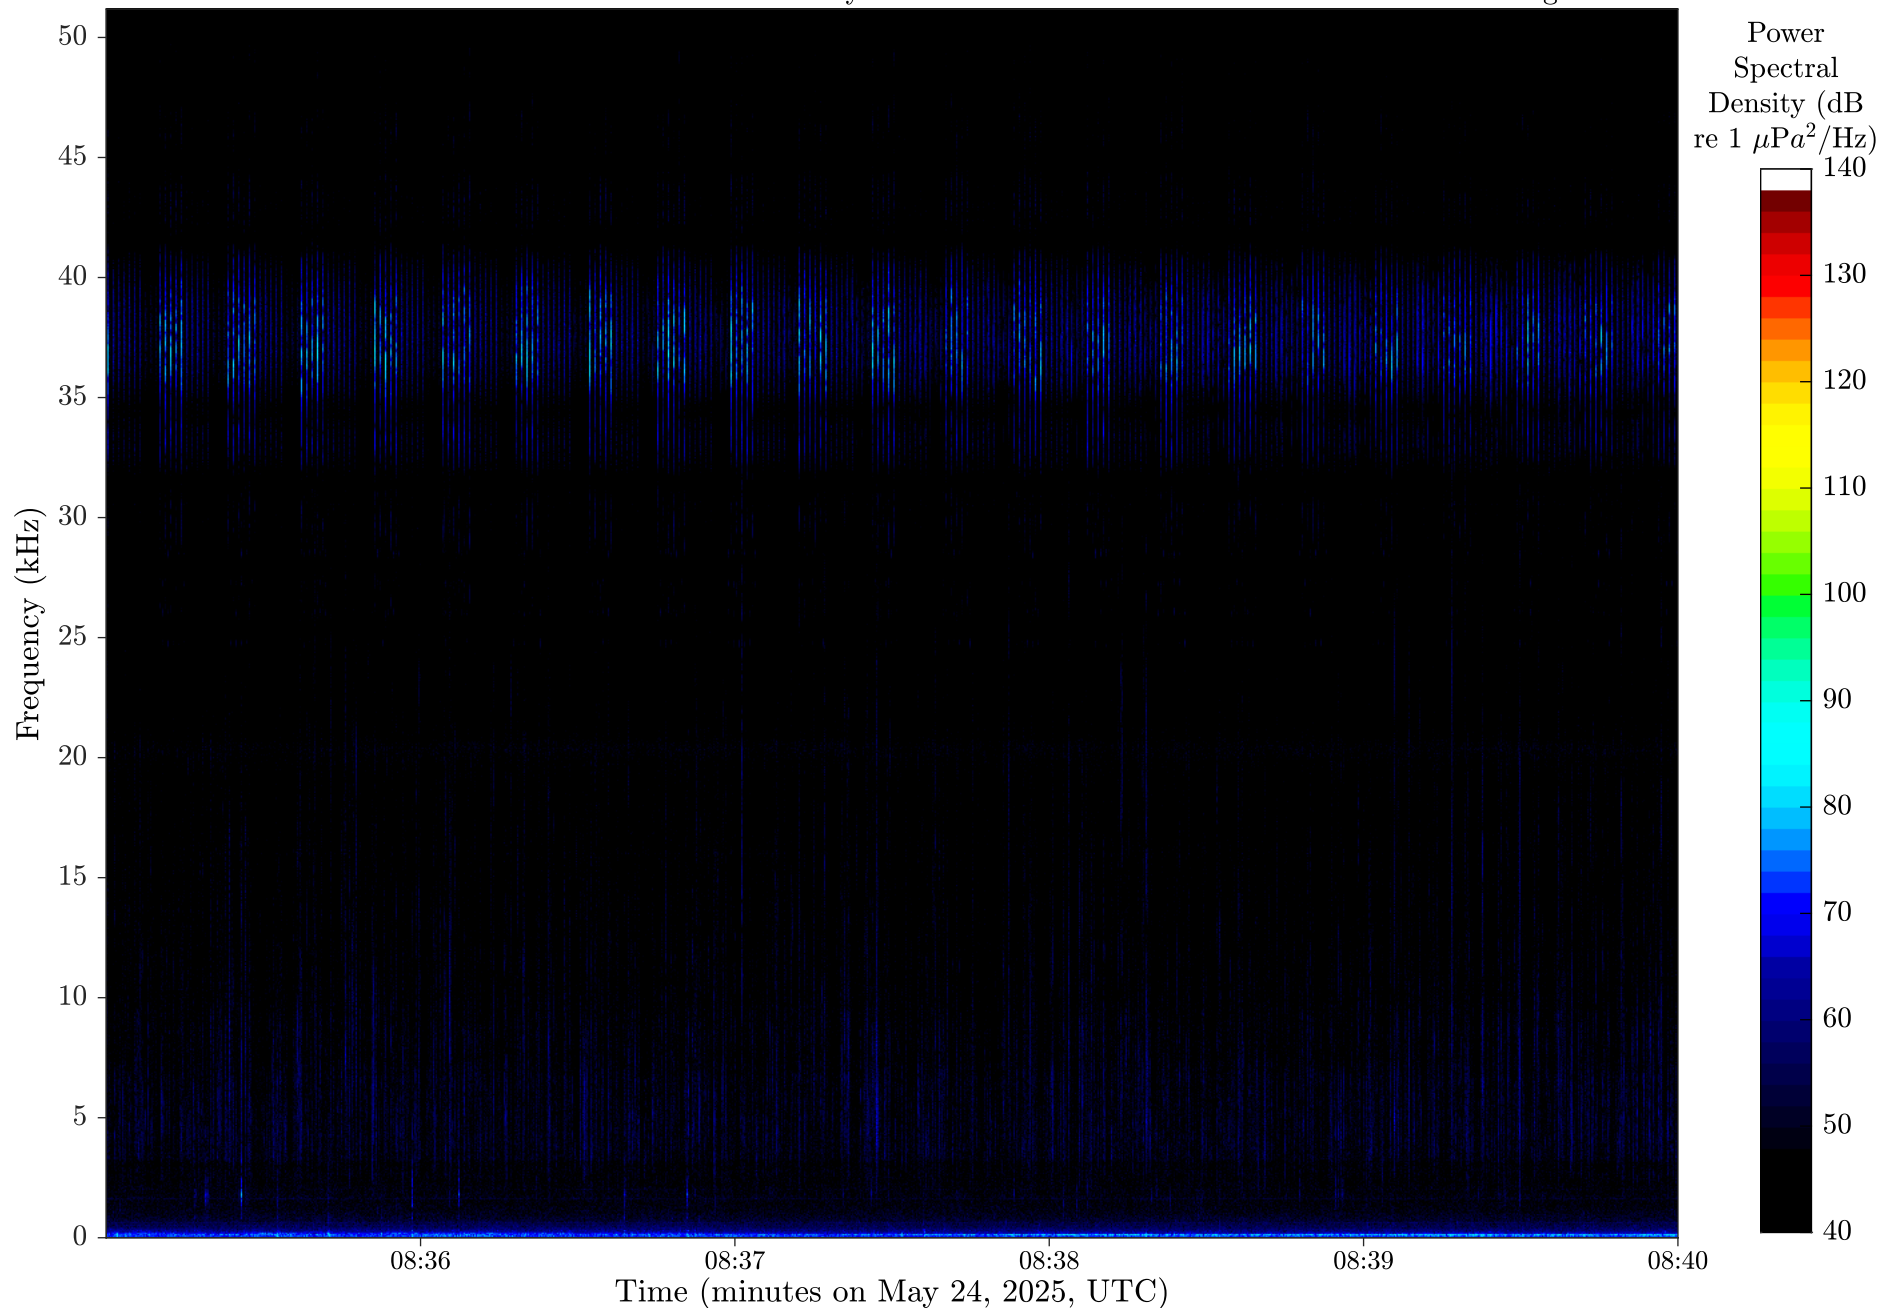

Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:33:28 UTC

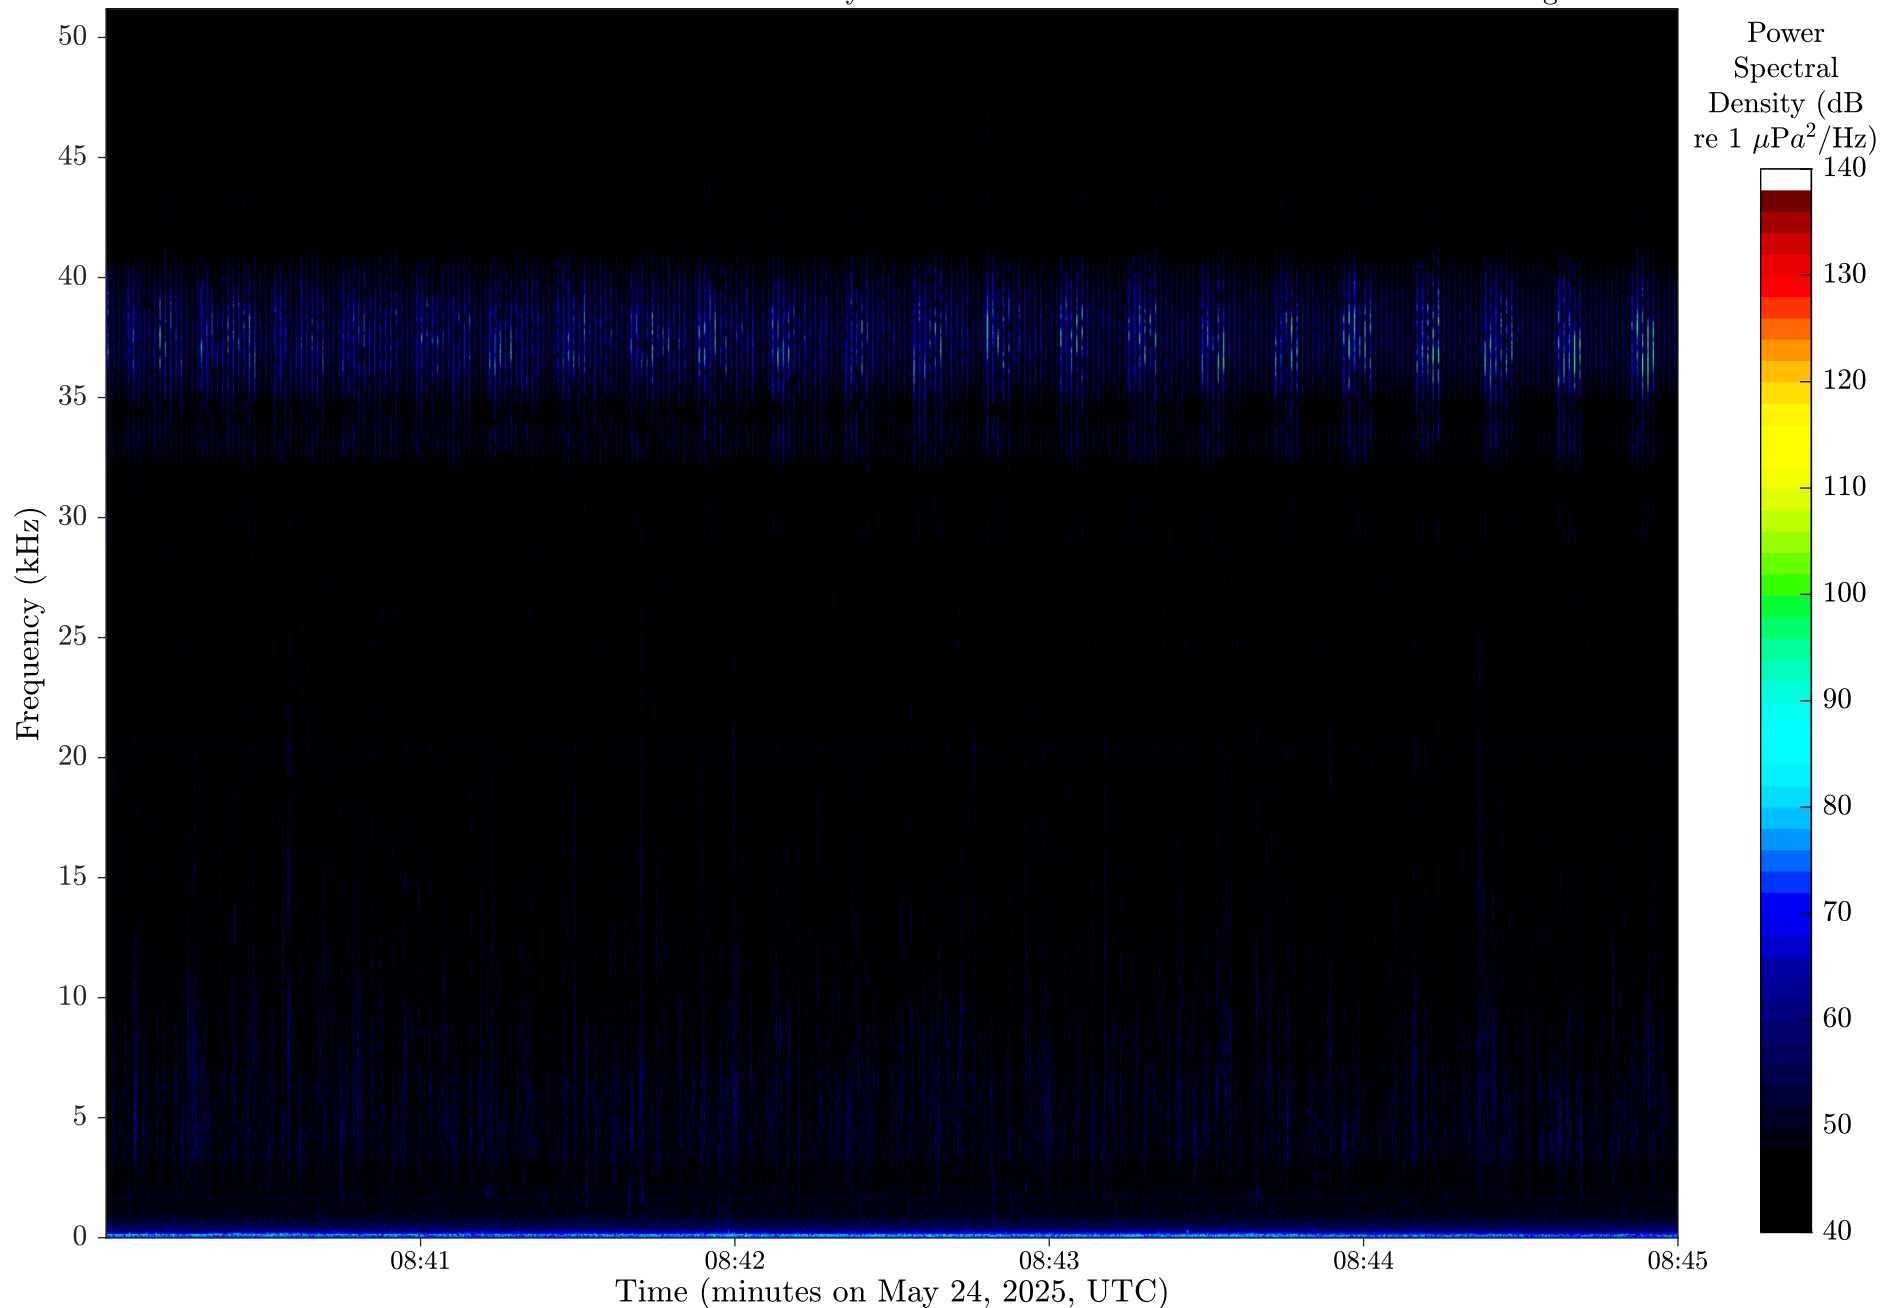


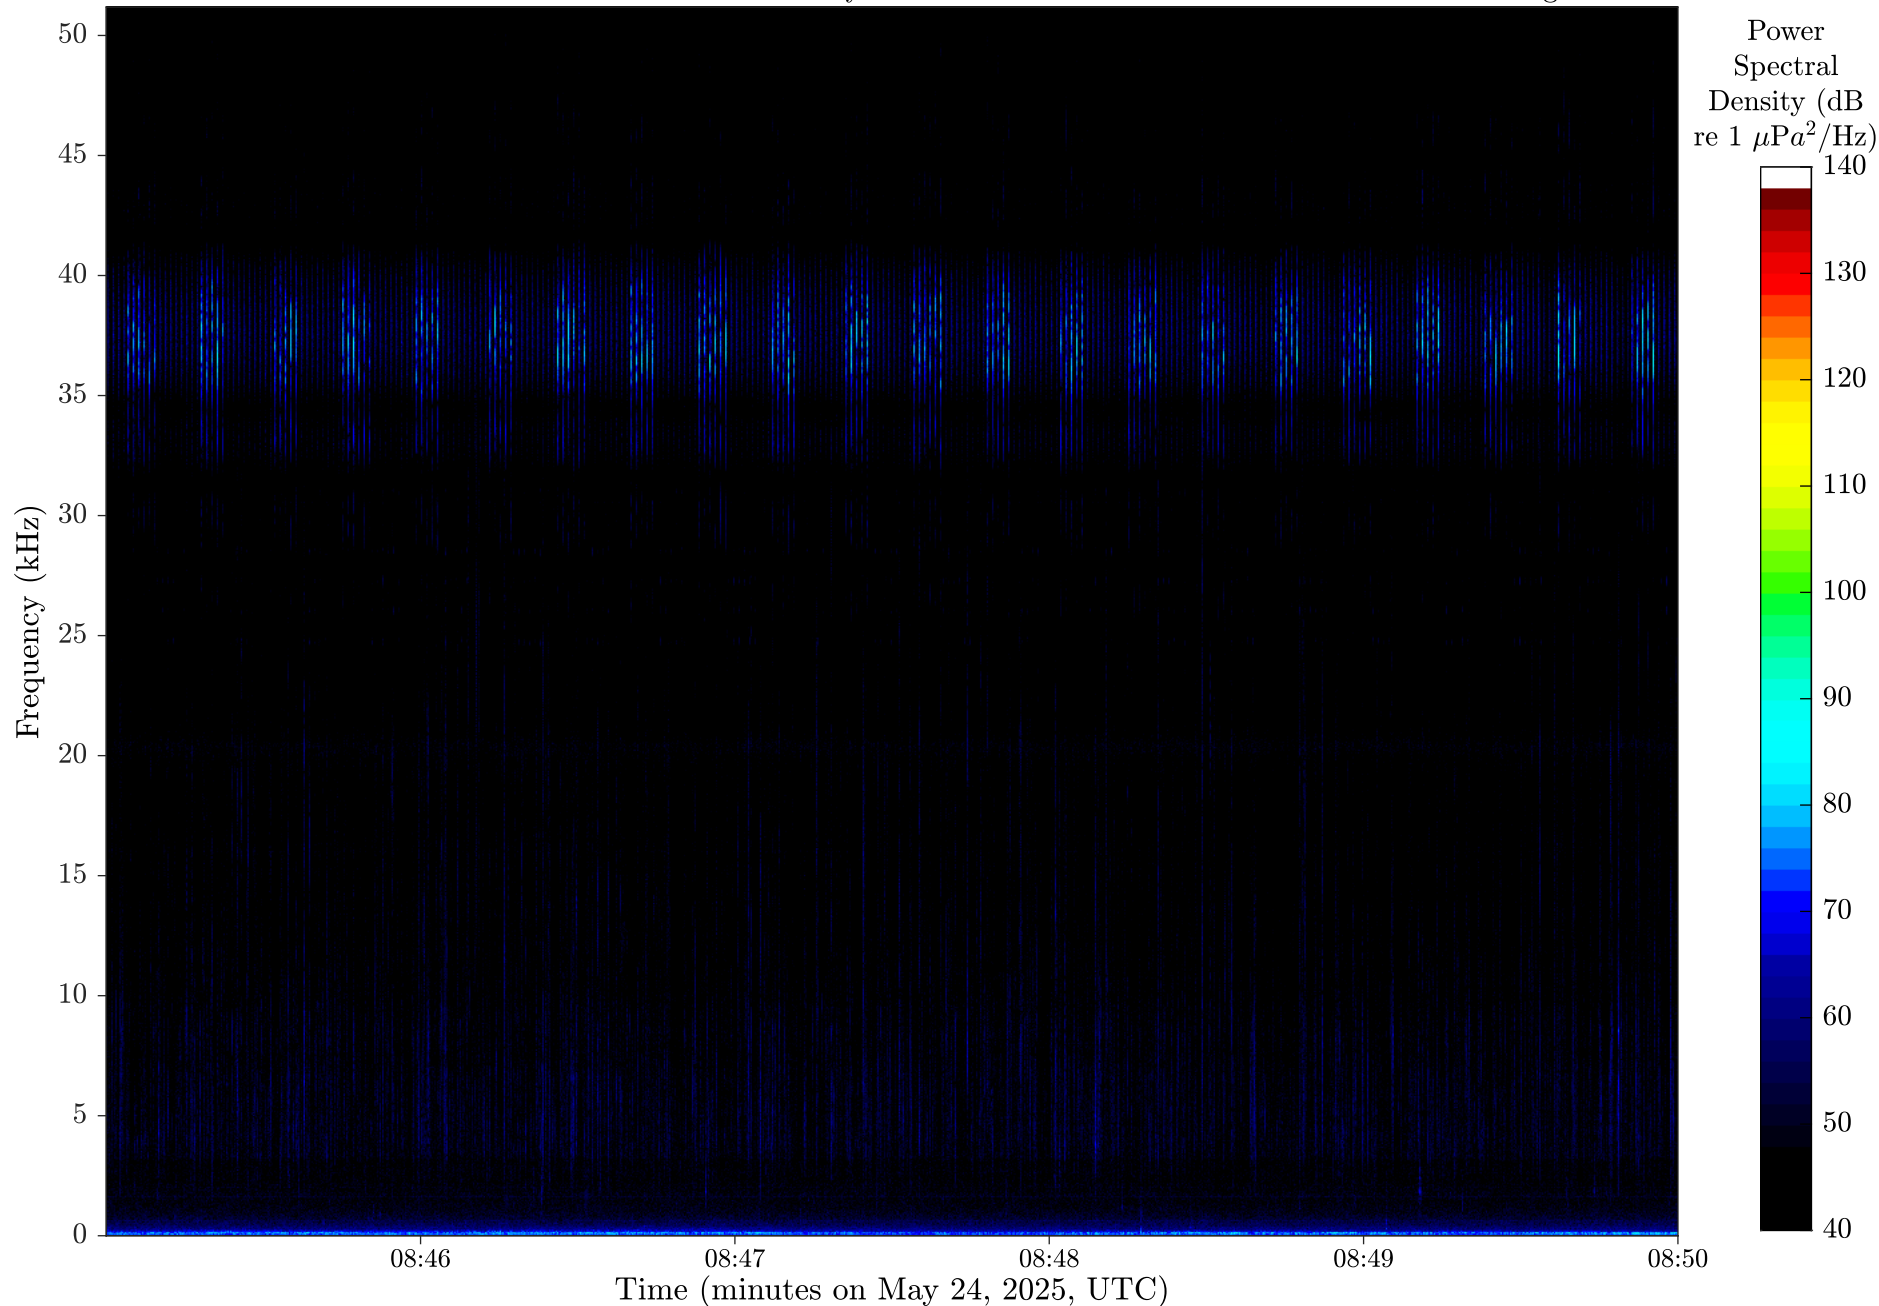

Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:33:44 UTC

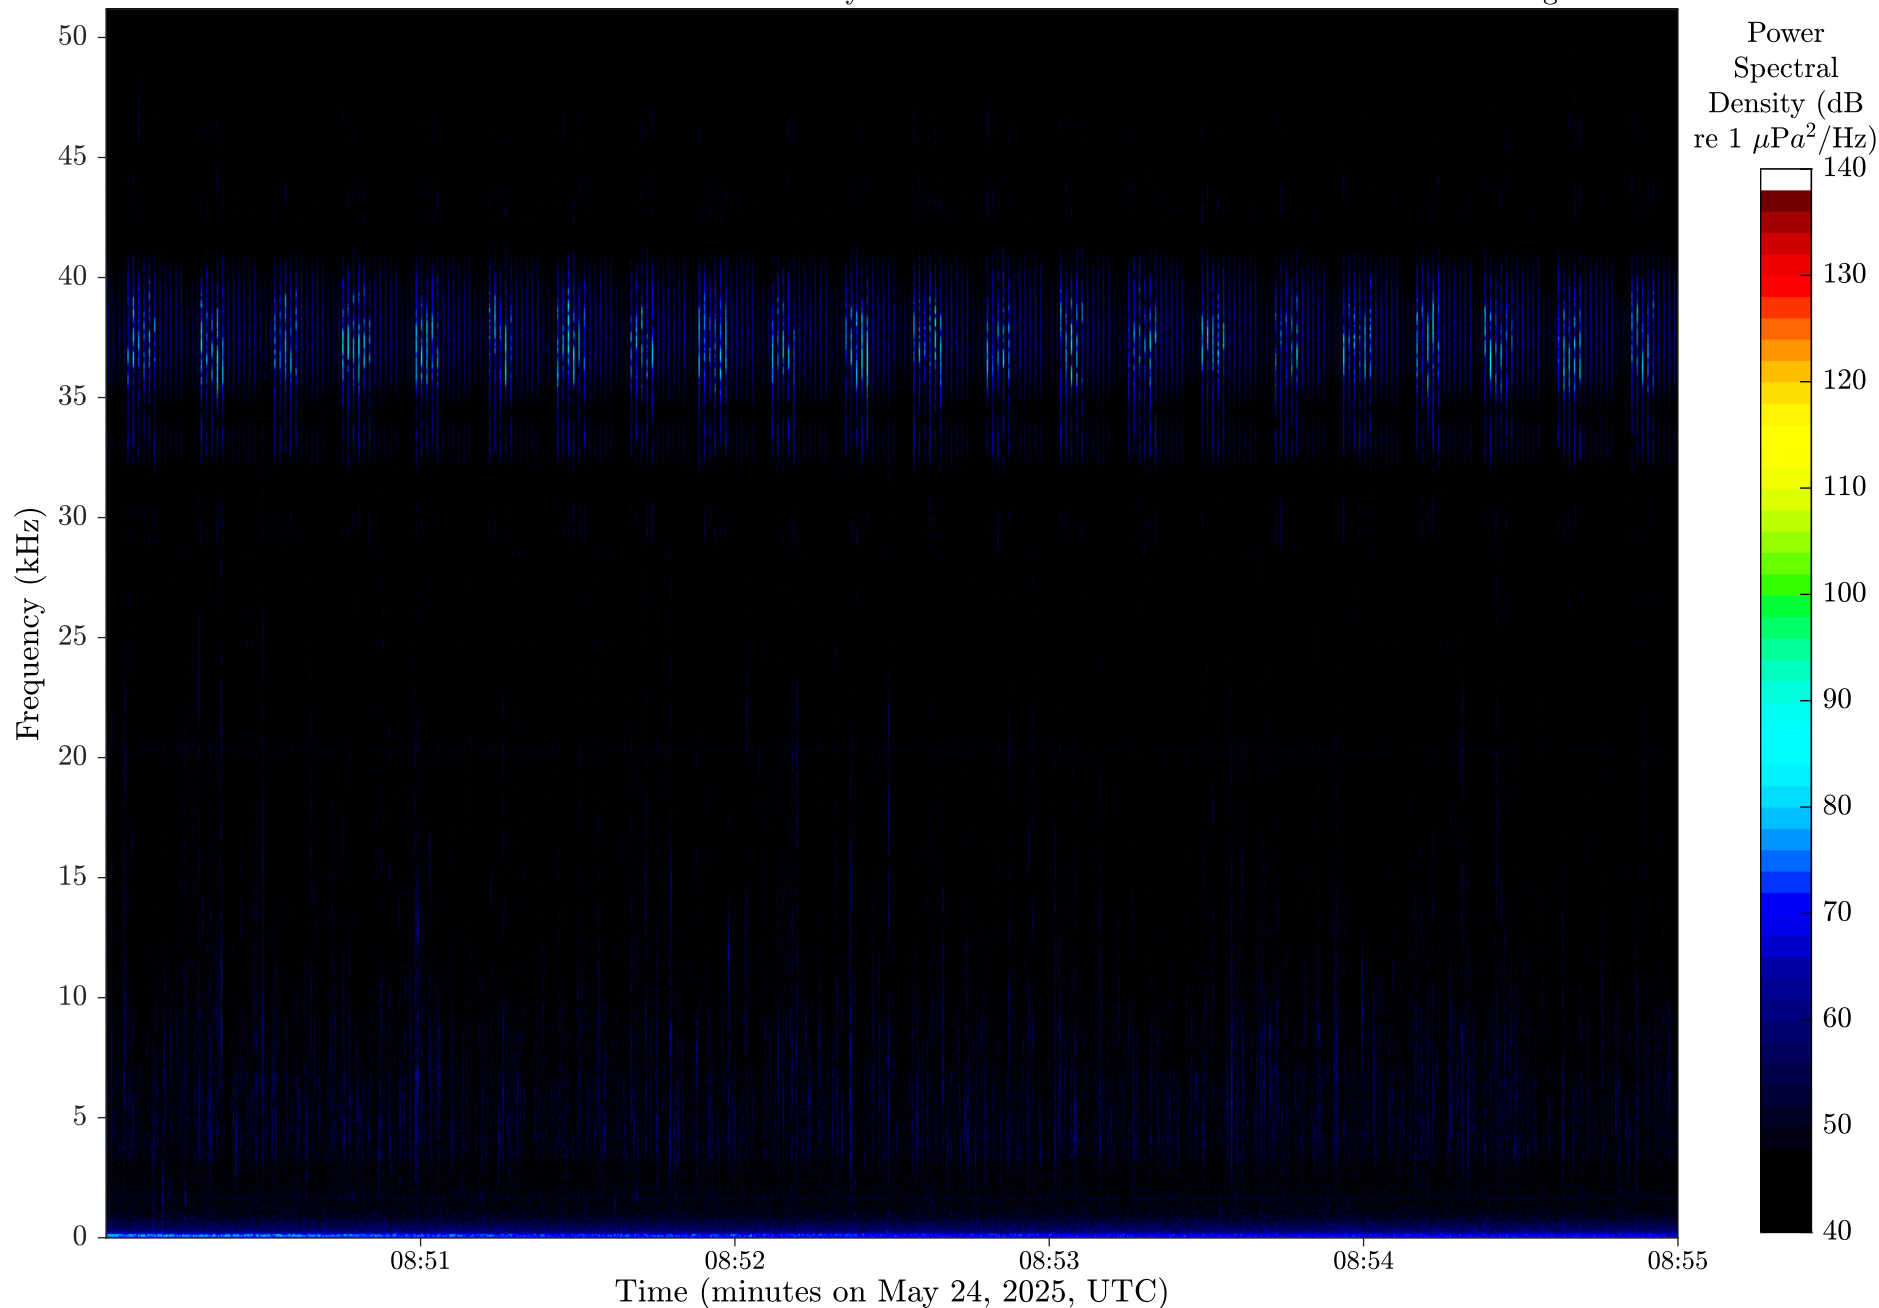

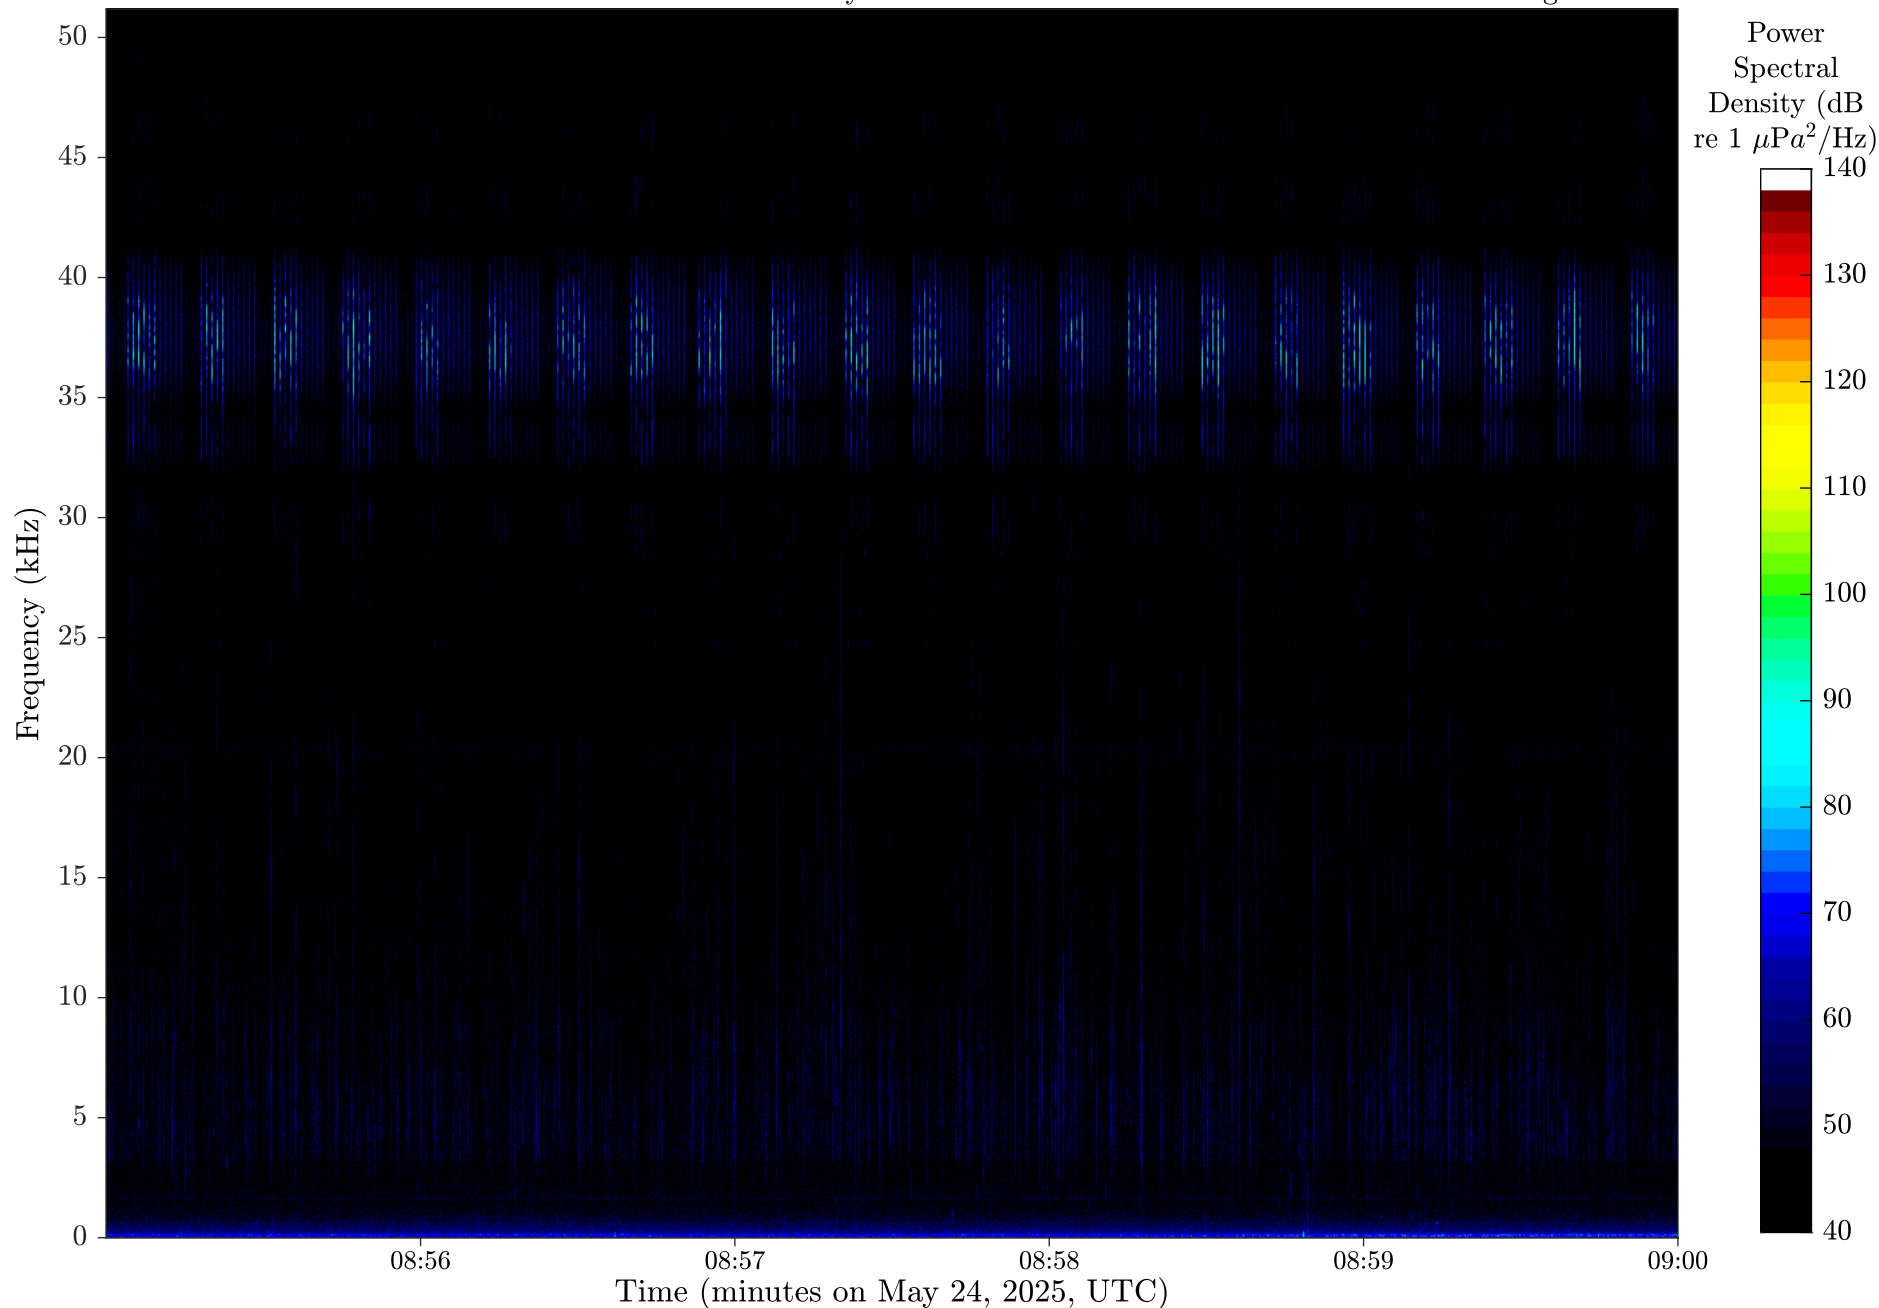


Comments: 36.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:00 UTC

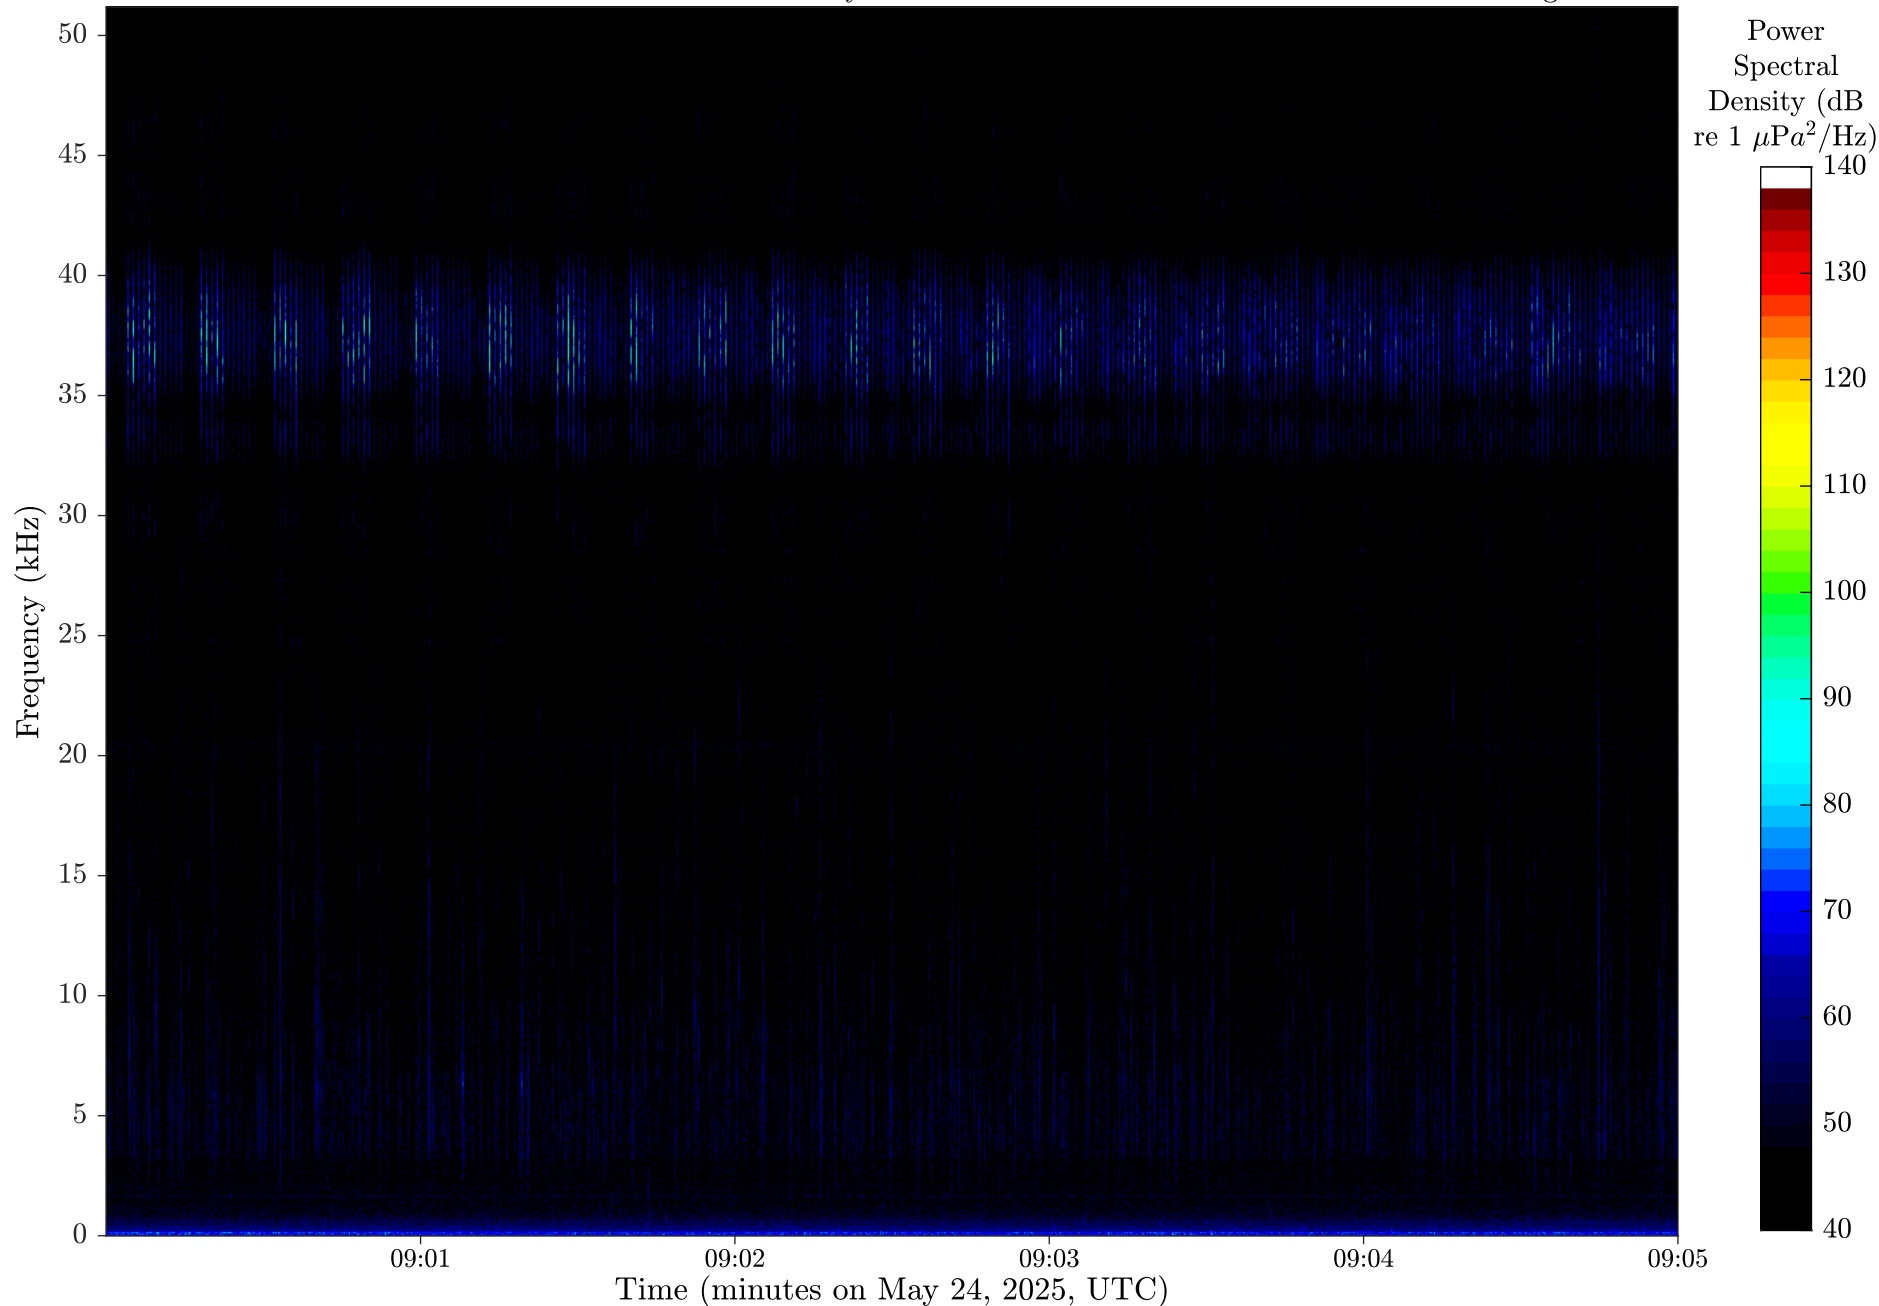


Comments: 35.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:07 UTC

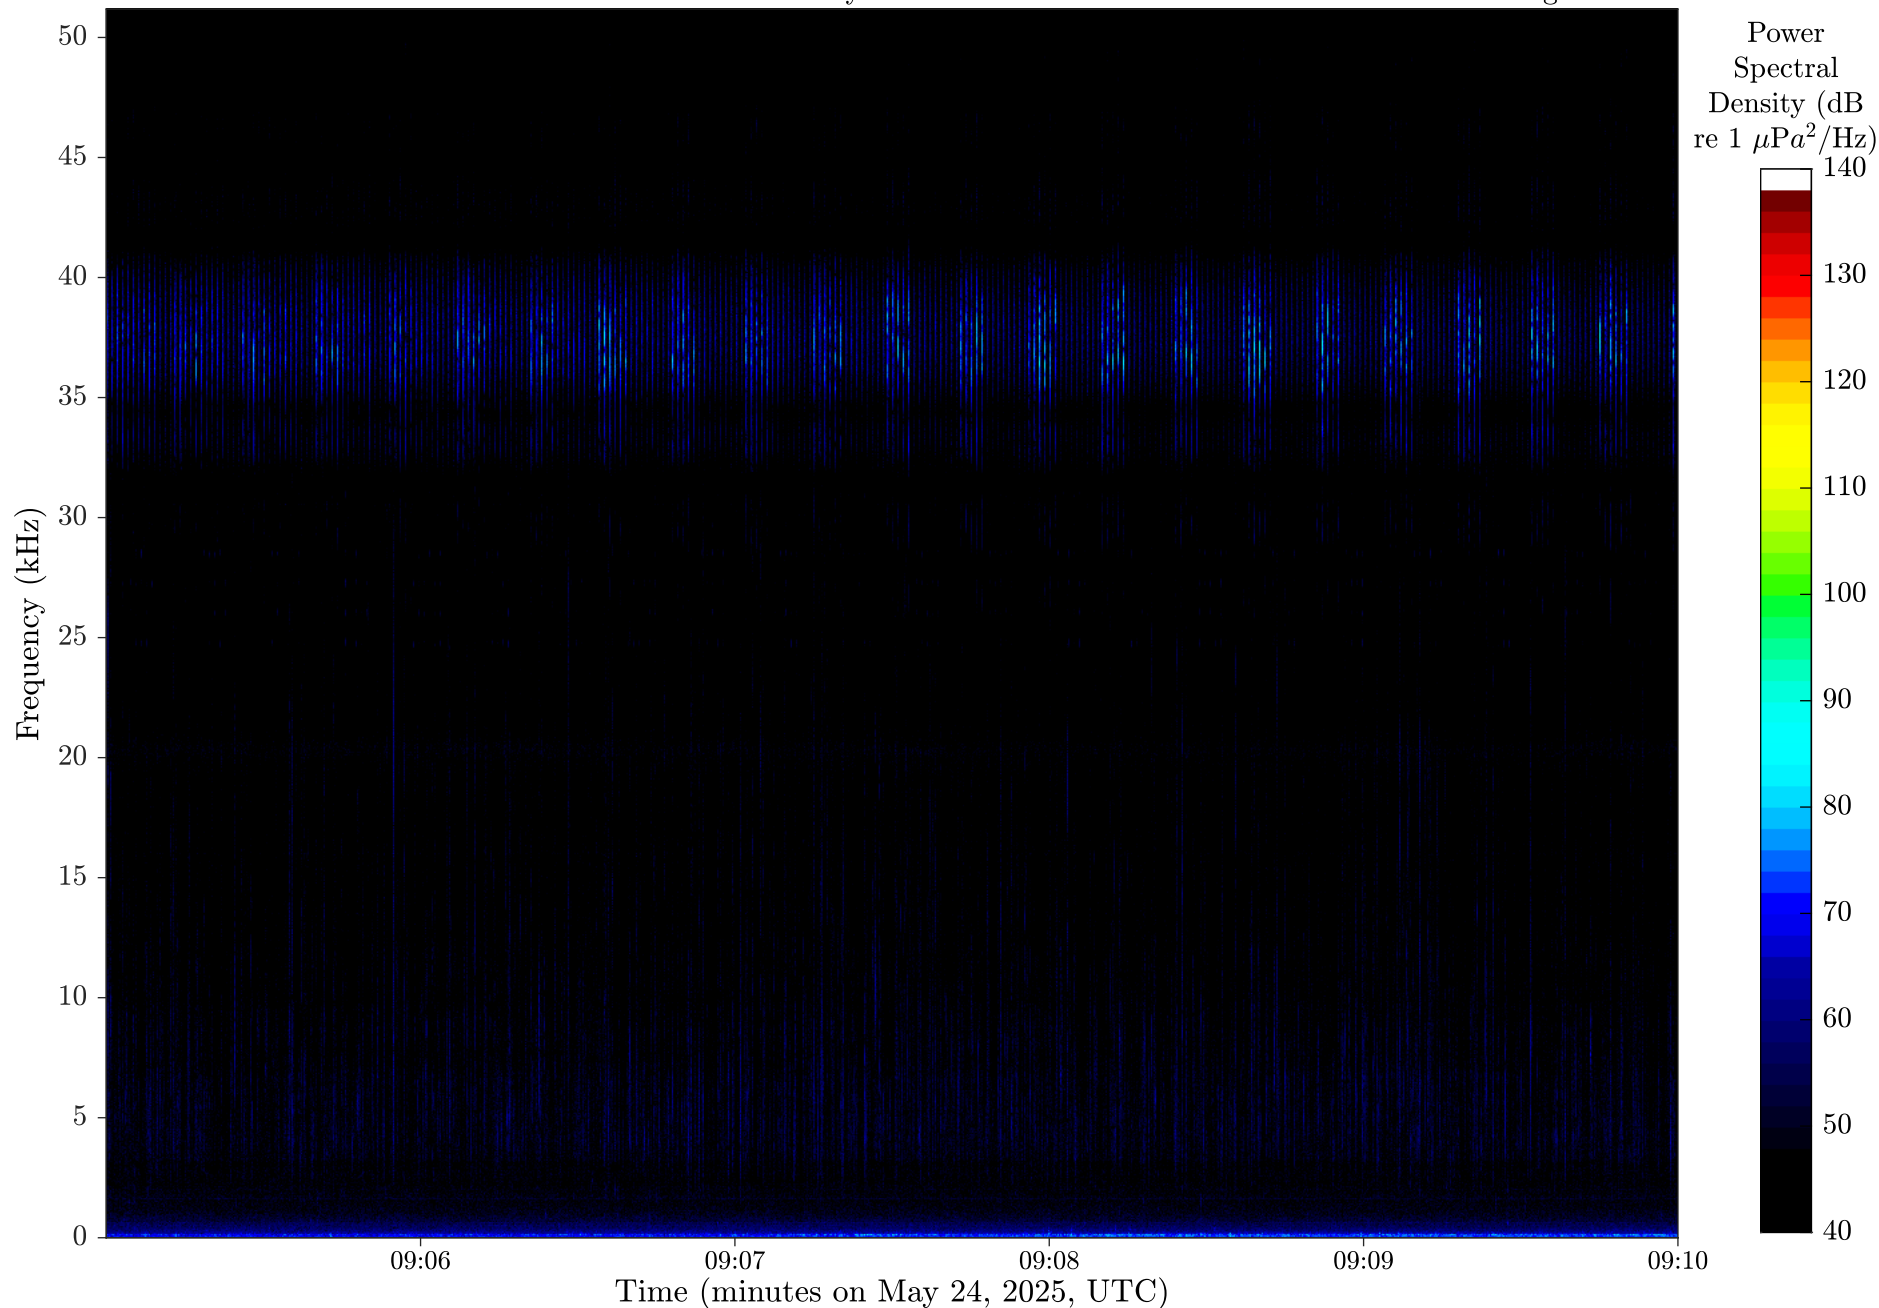


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:34:16 UTC

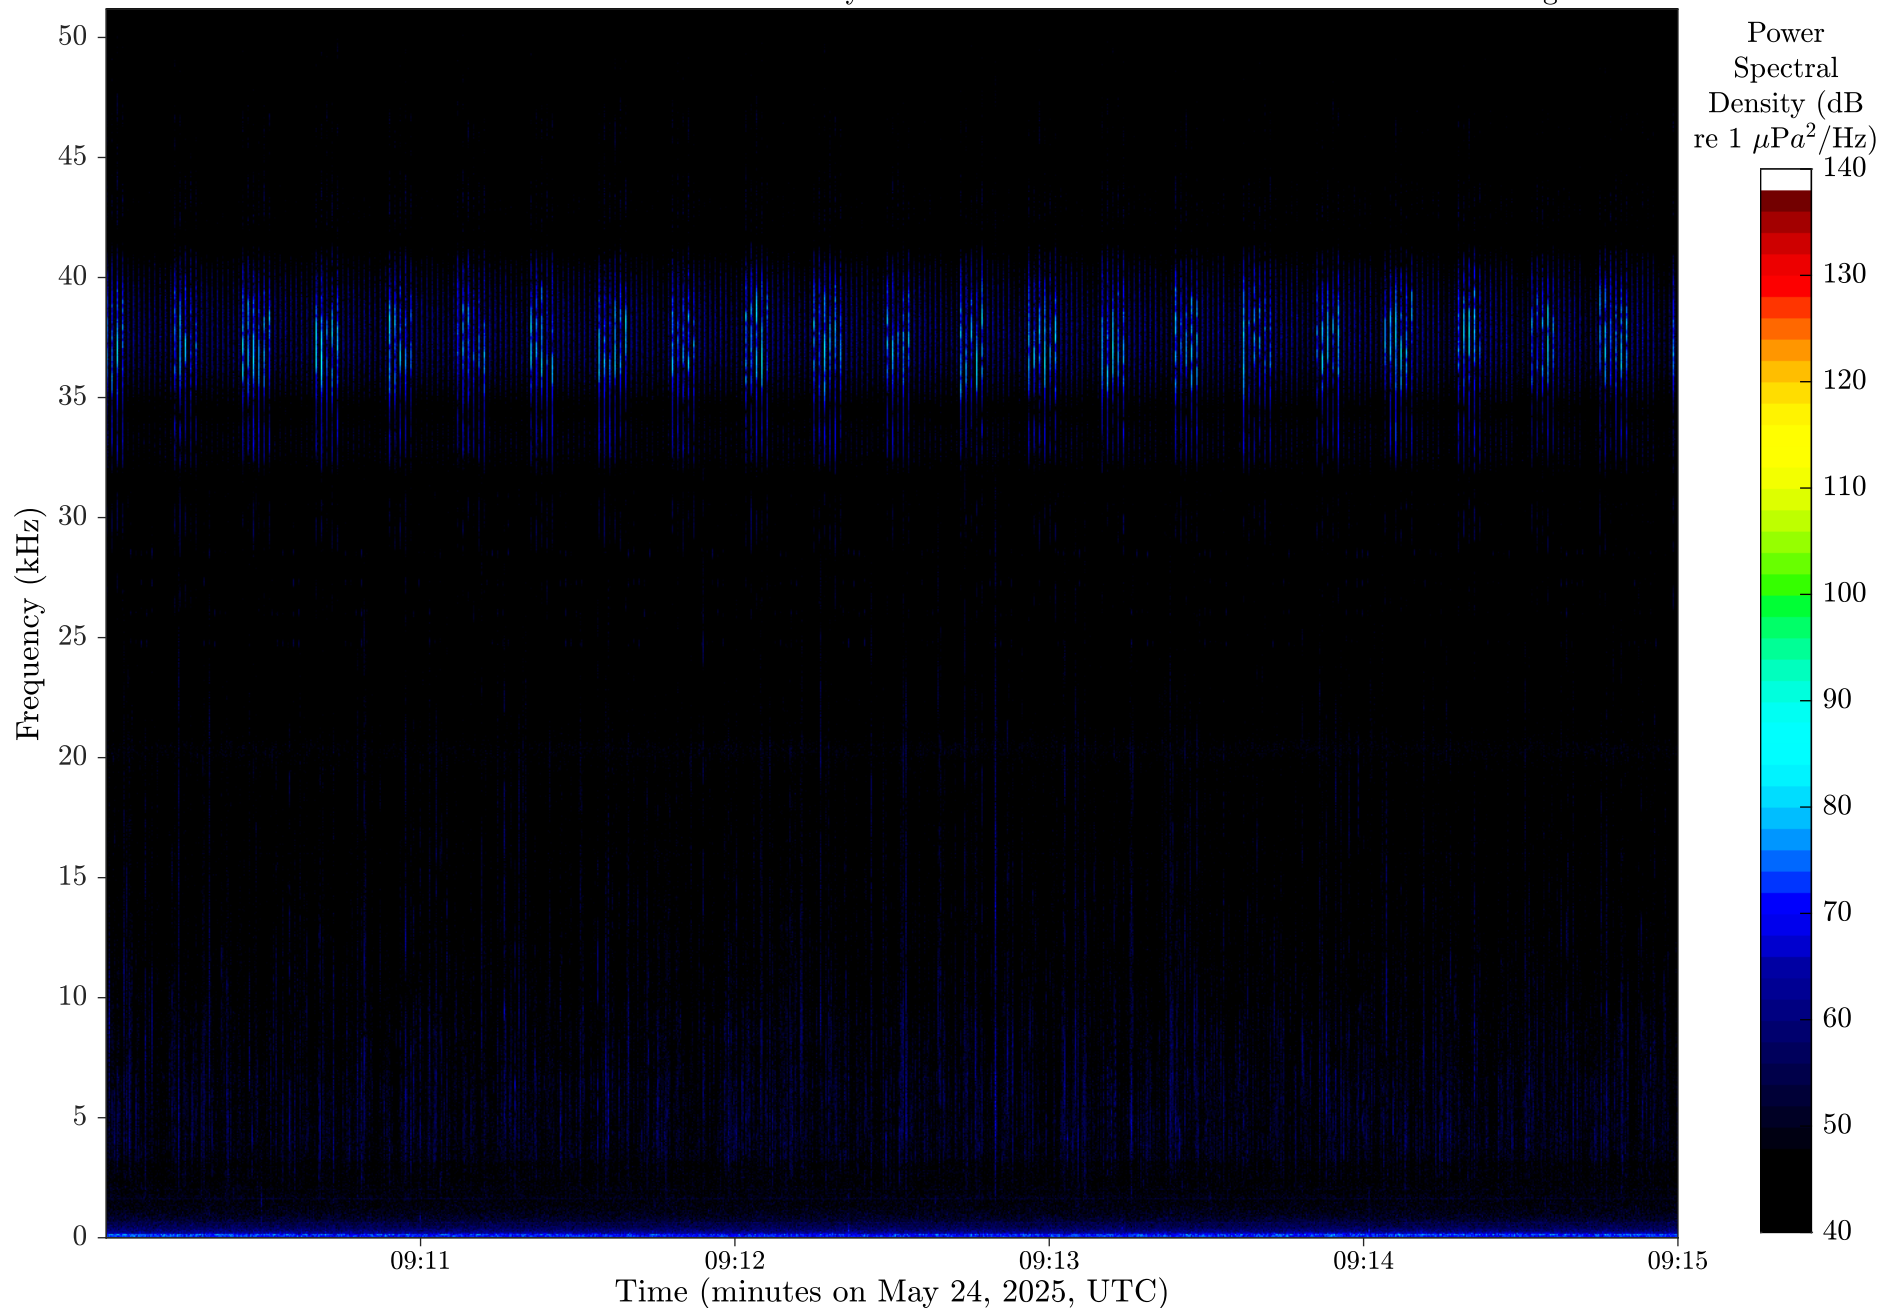

Comments: 35.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:34:23 UTC

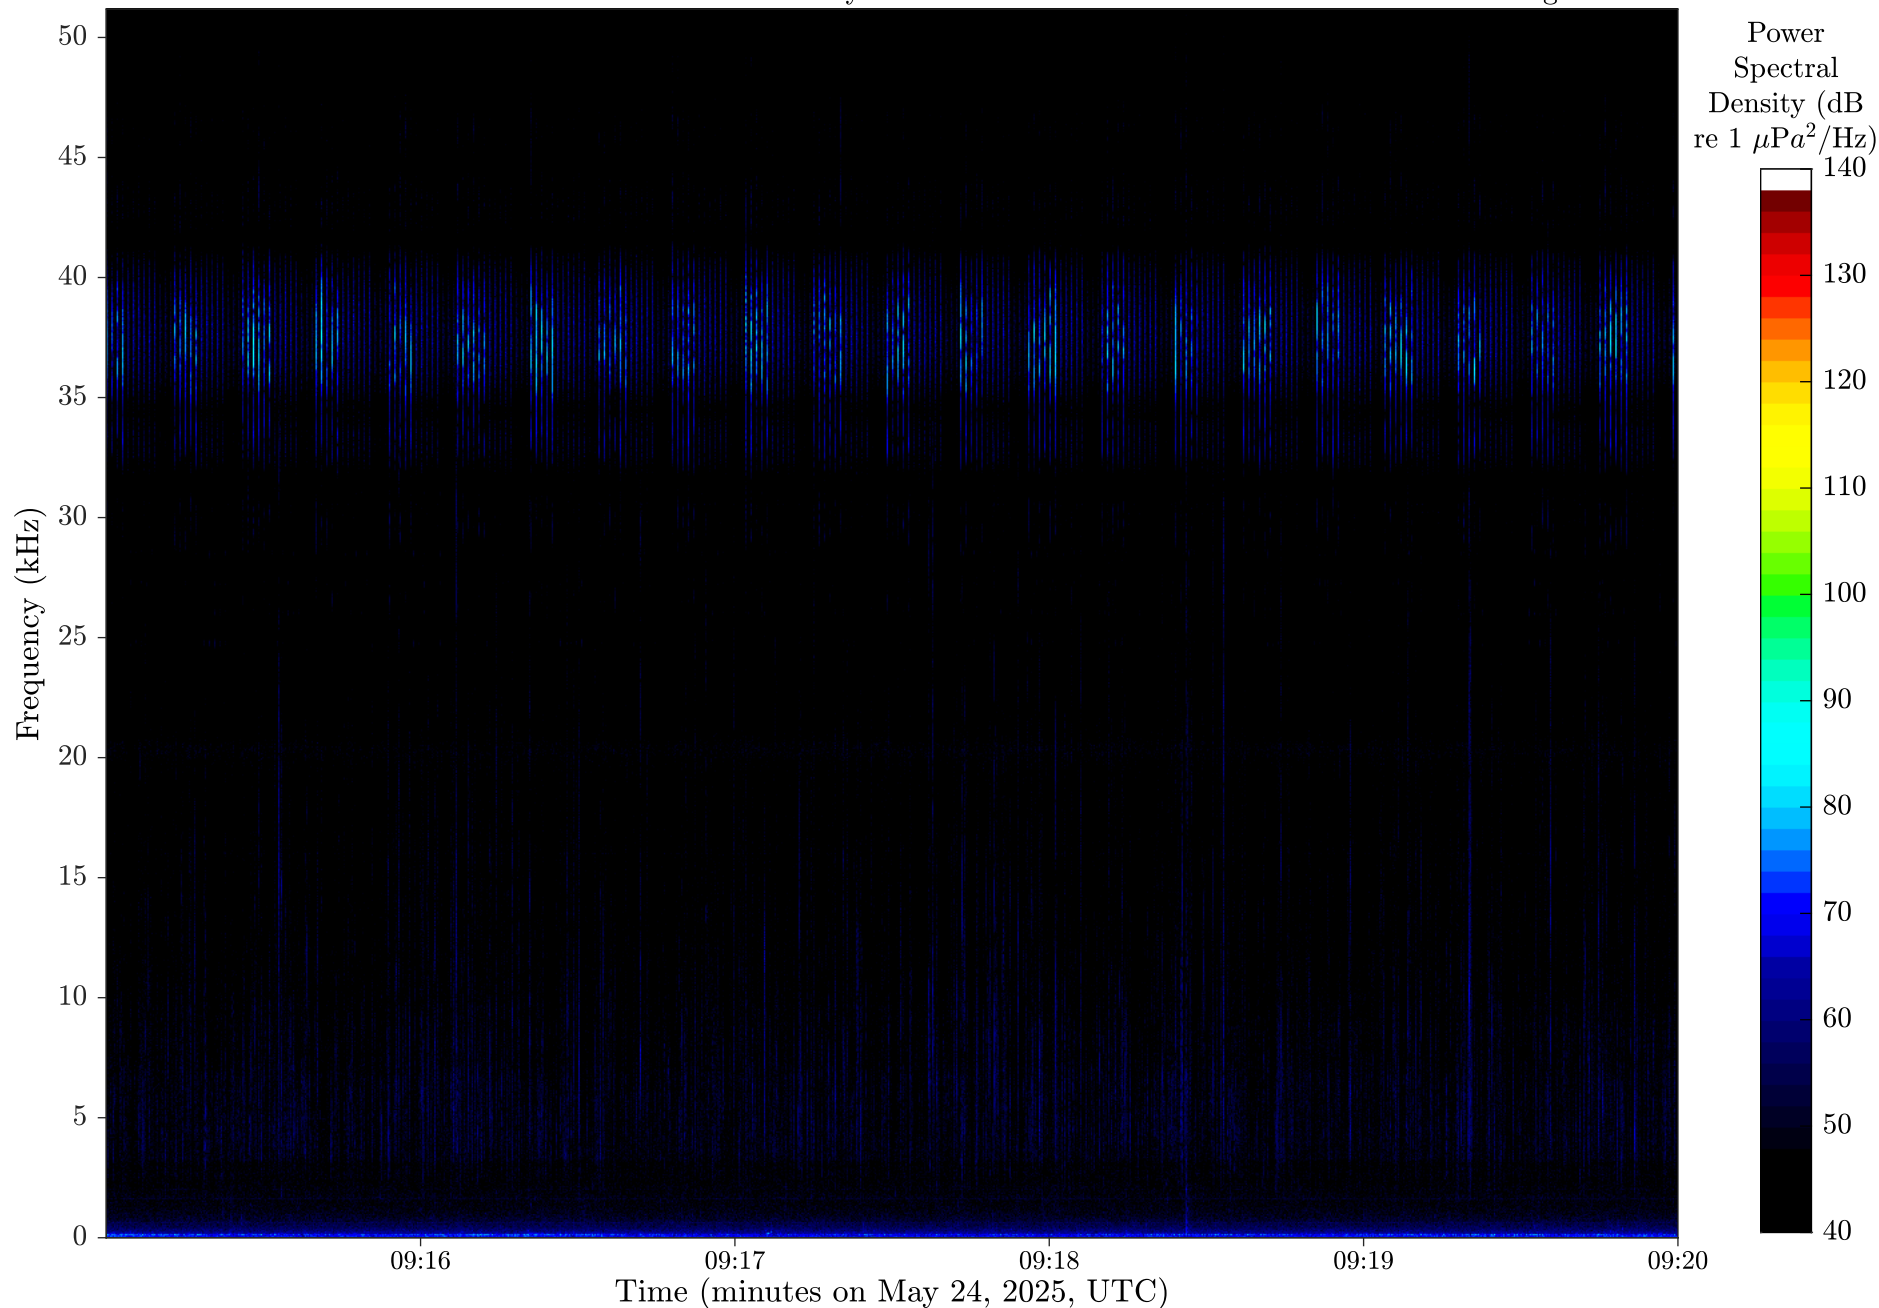

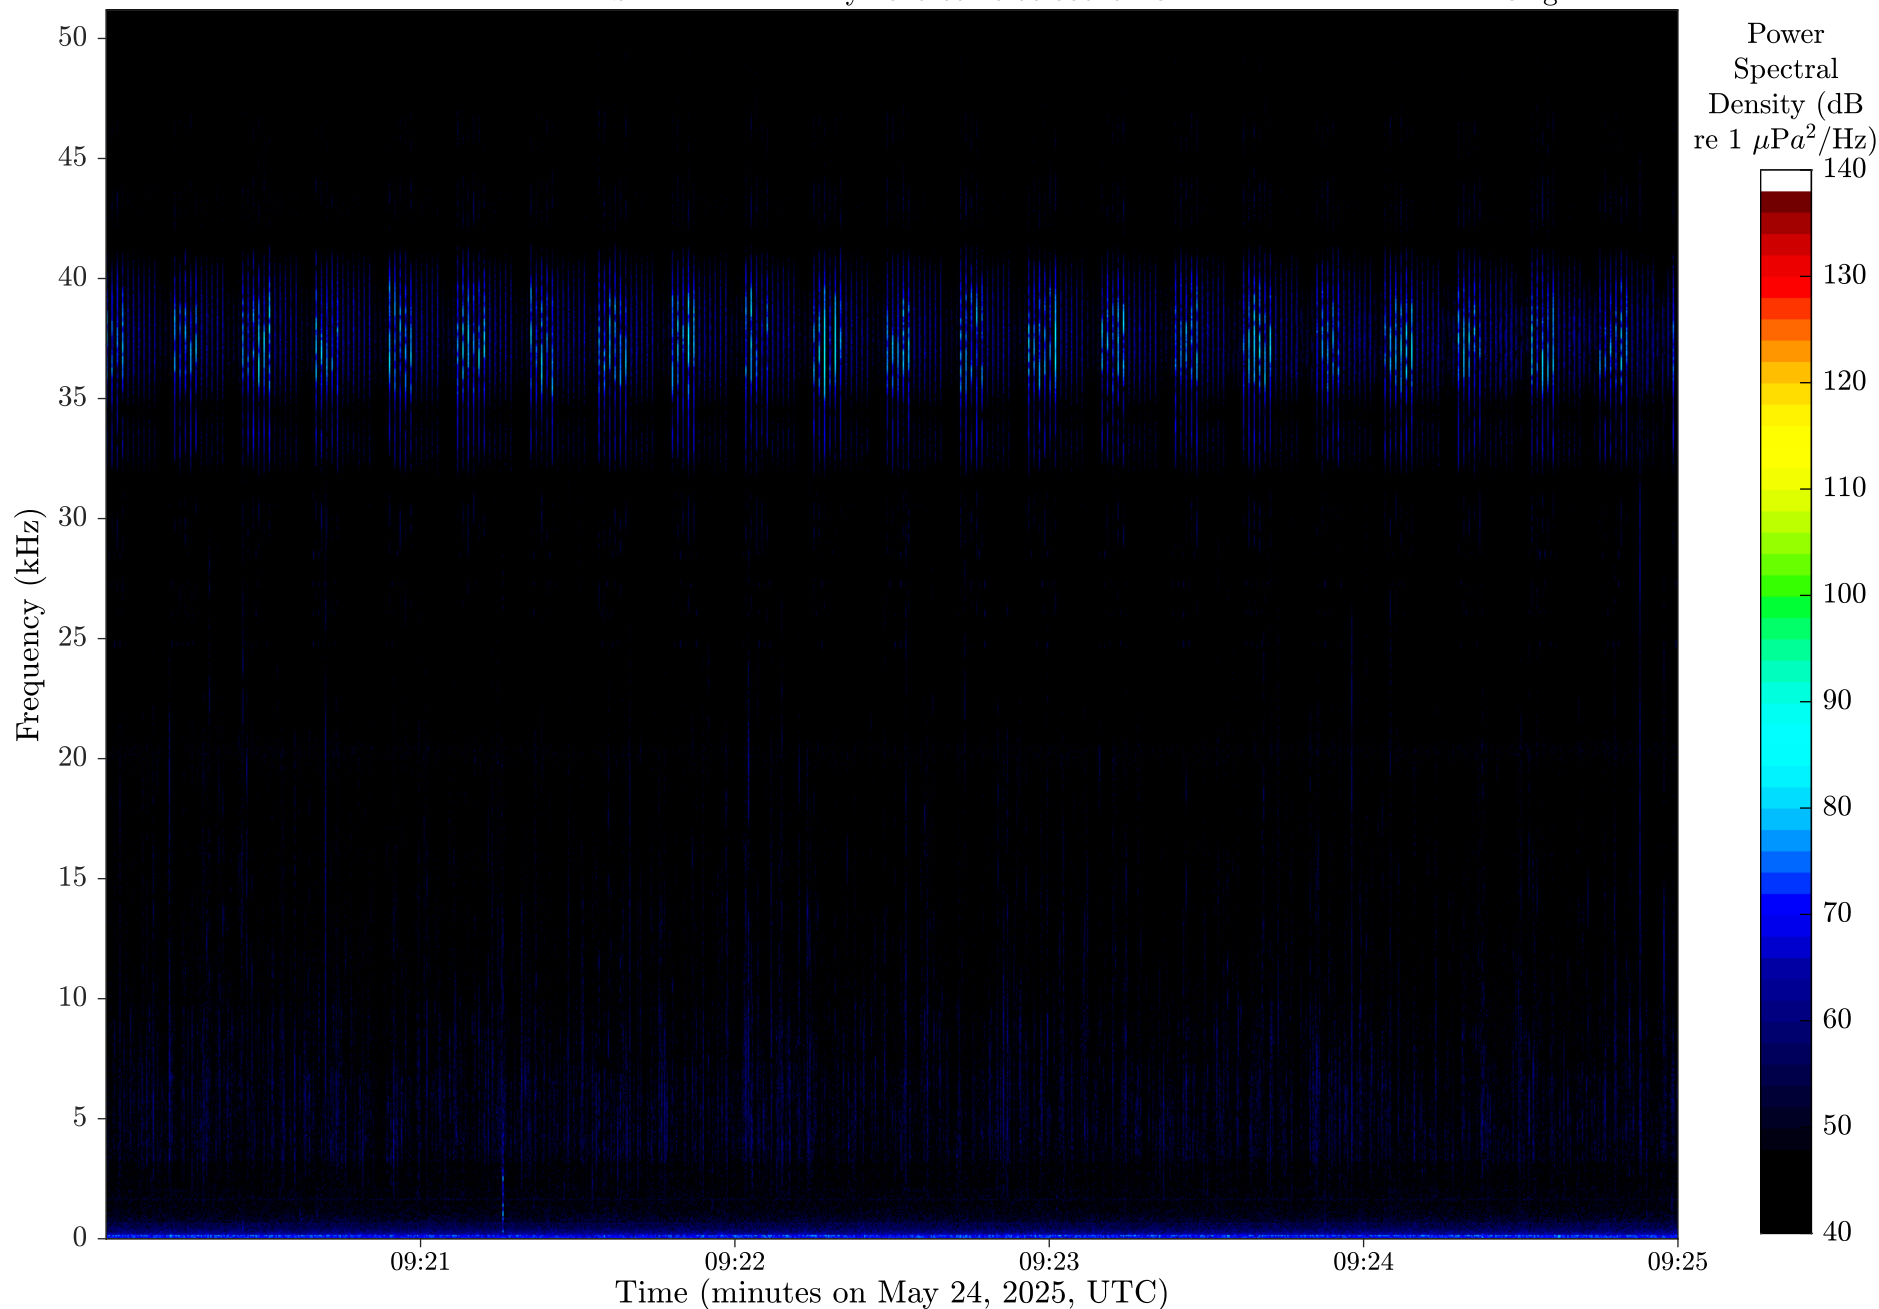


Comments: 35.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:34:39 UTC

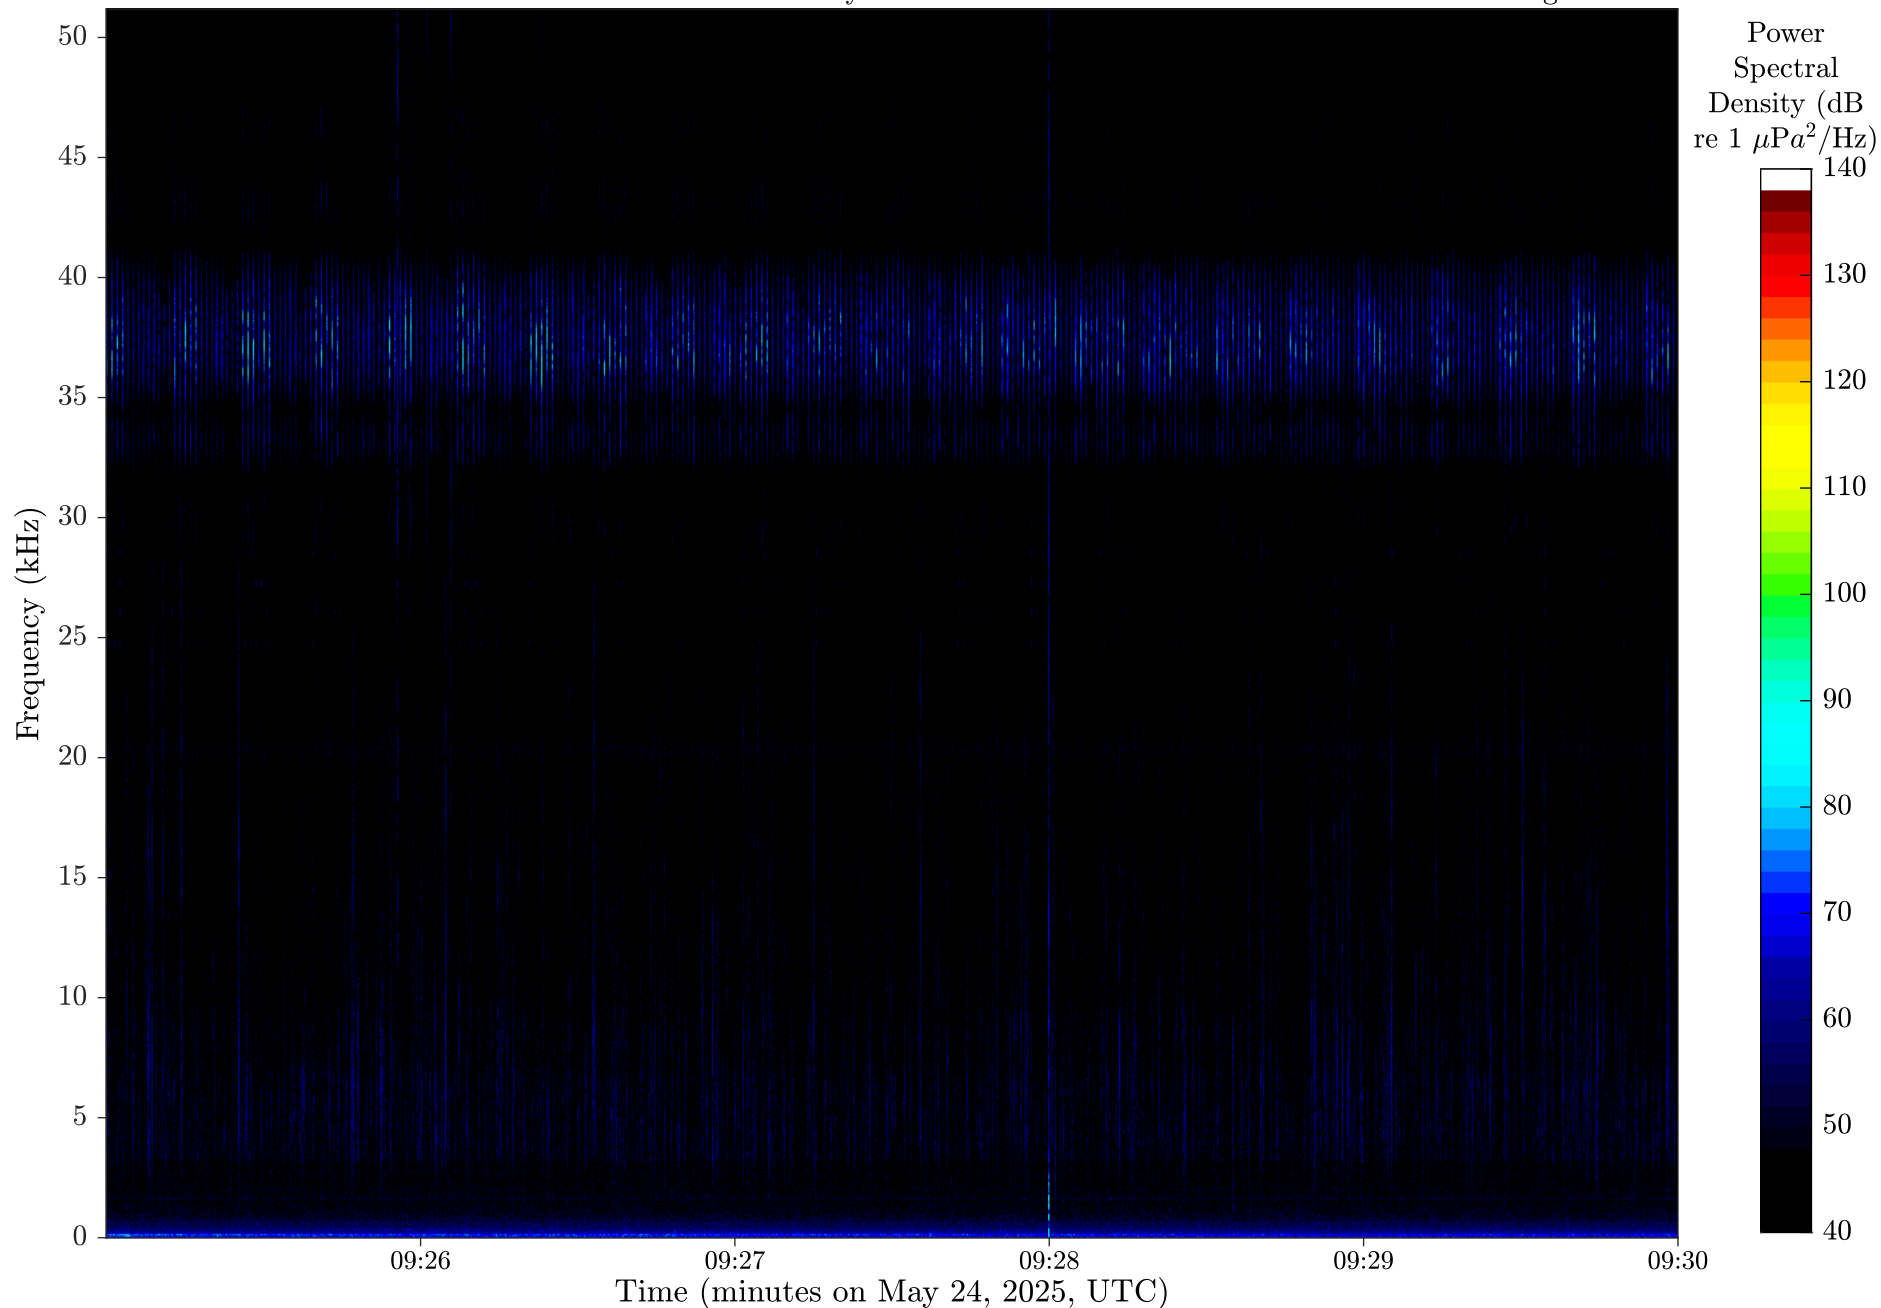


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:34:47 UTC

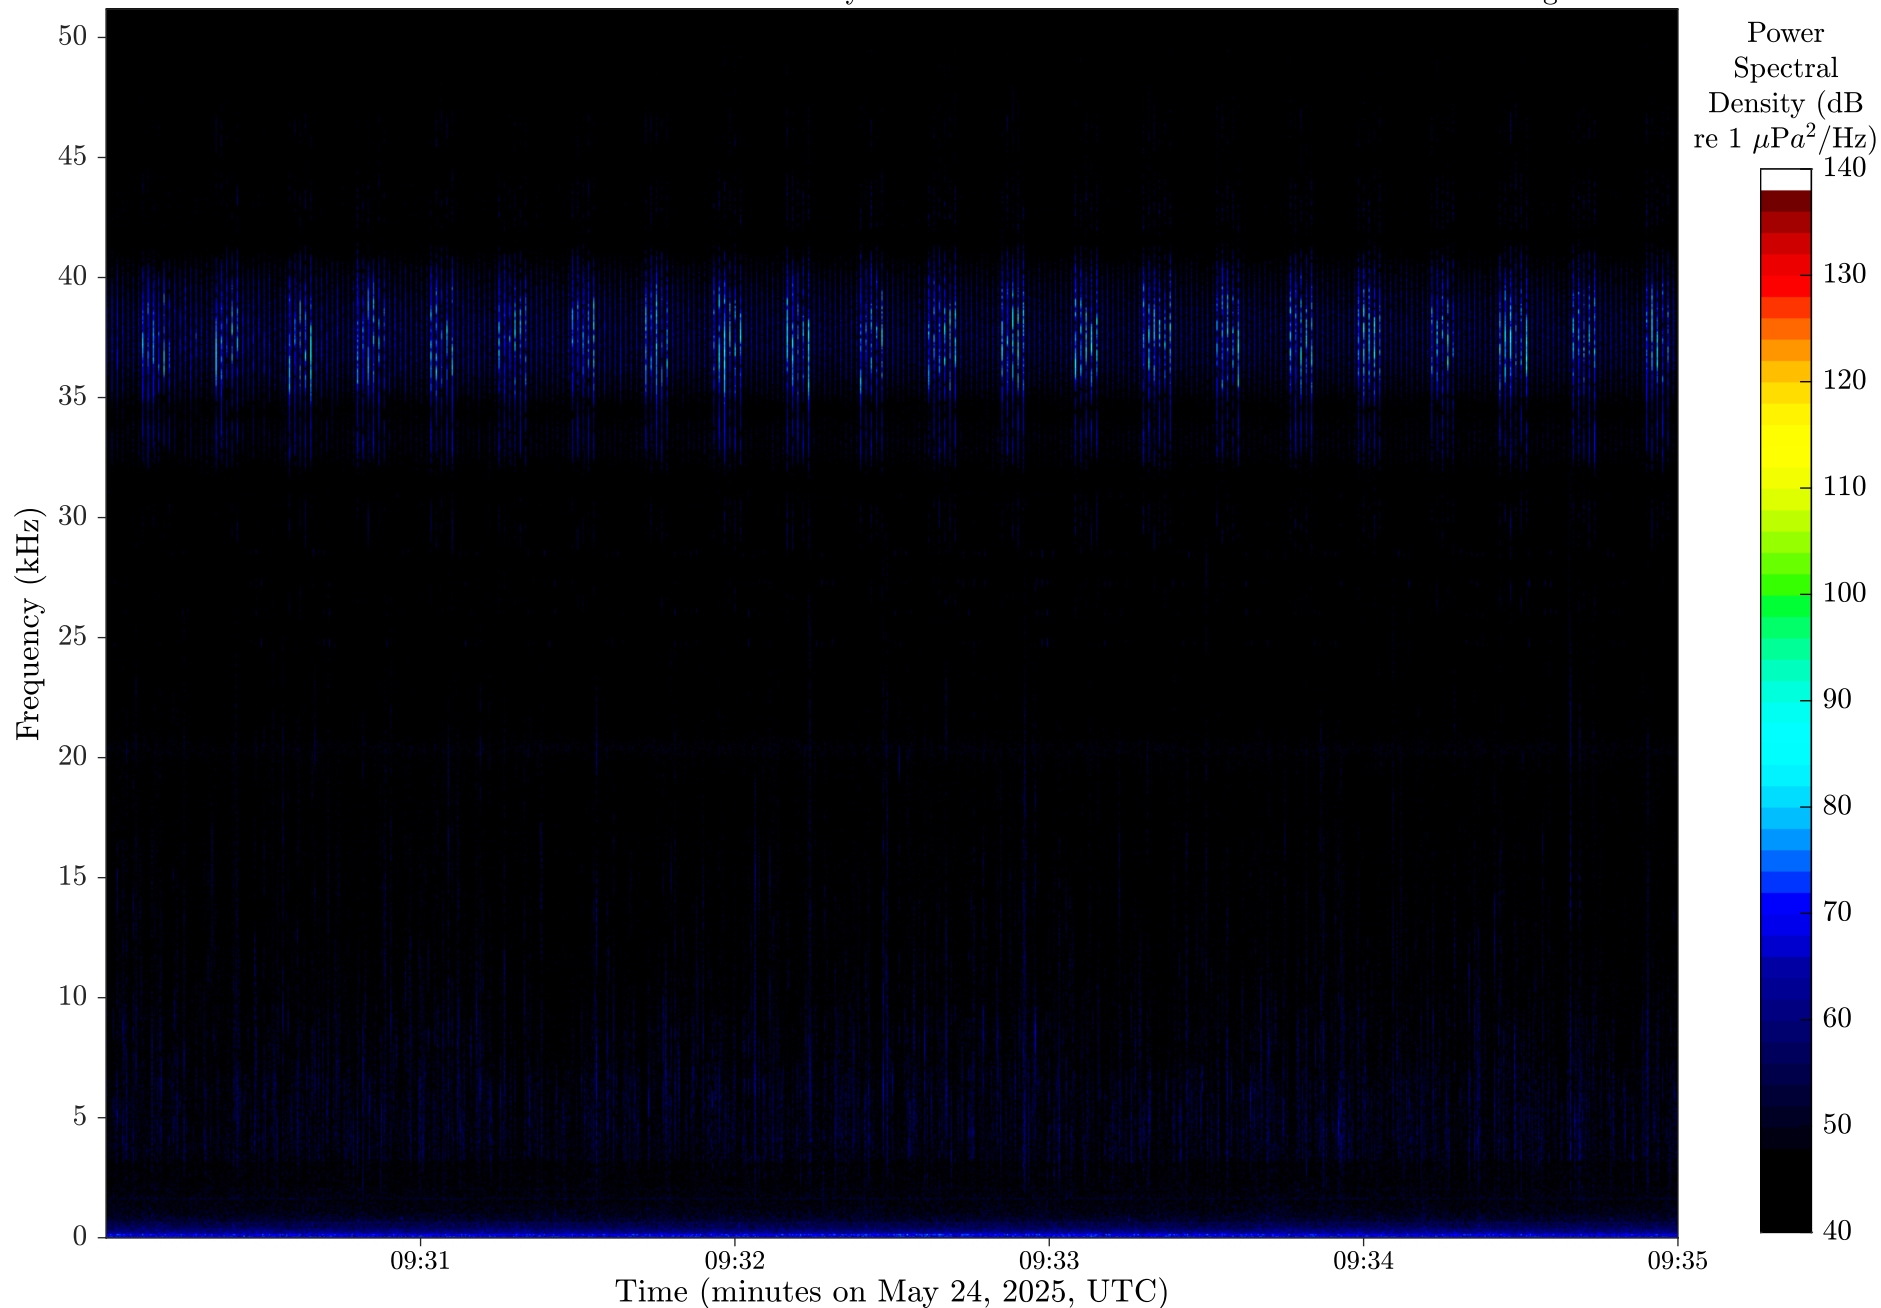

Comments: 35.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:34:54 UTC

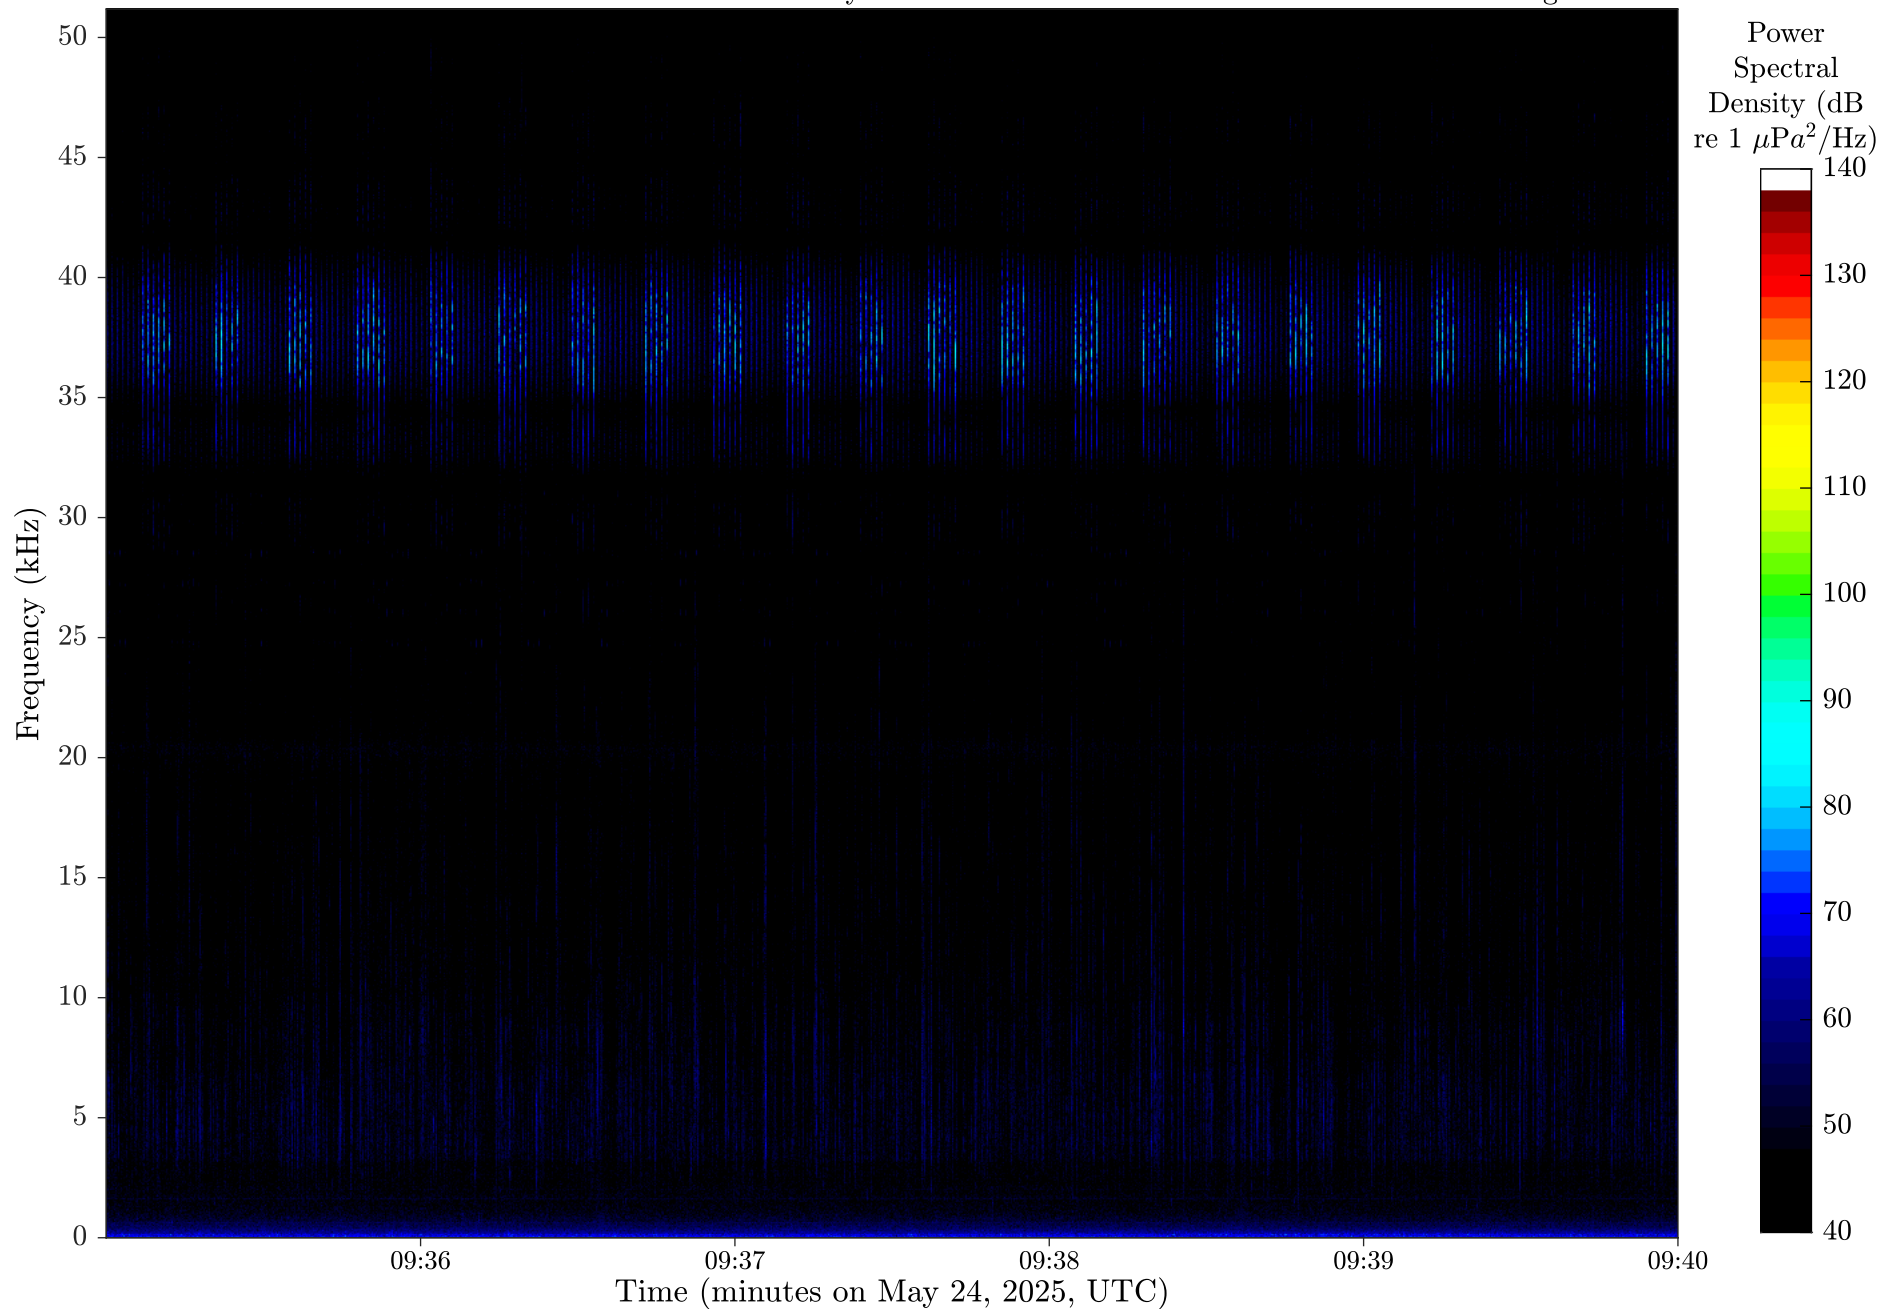

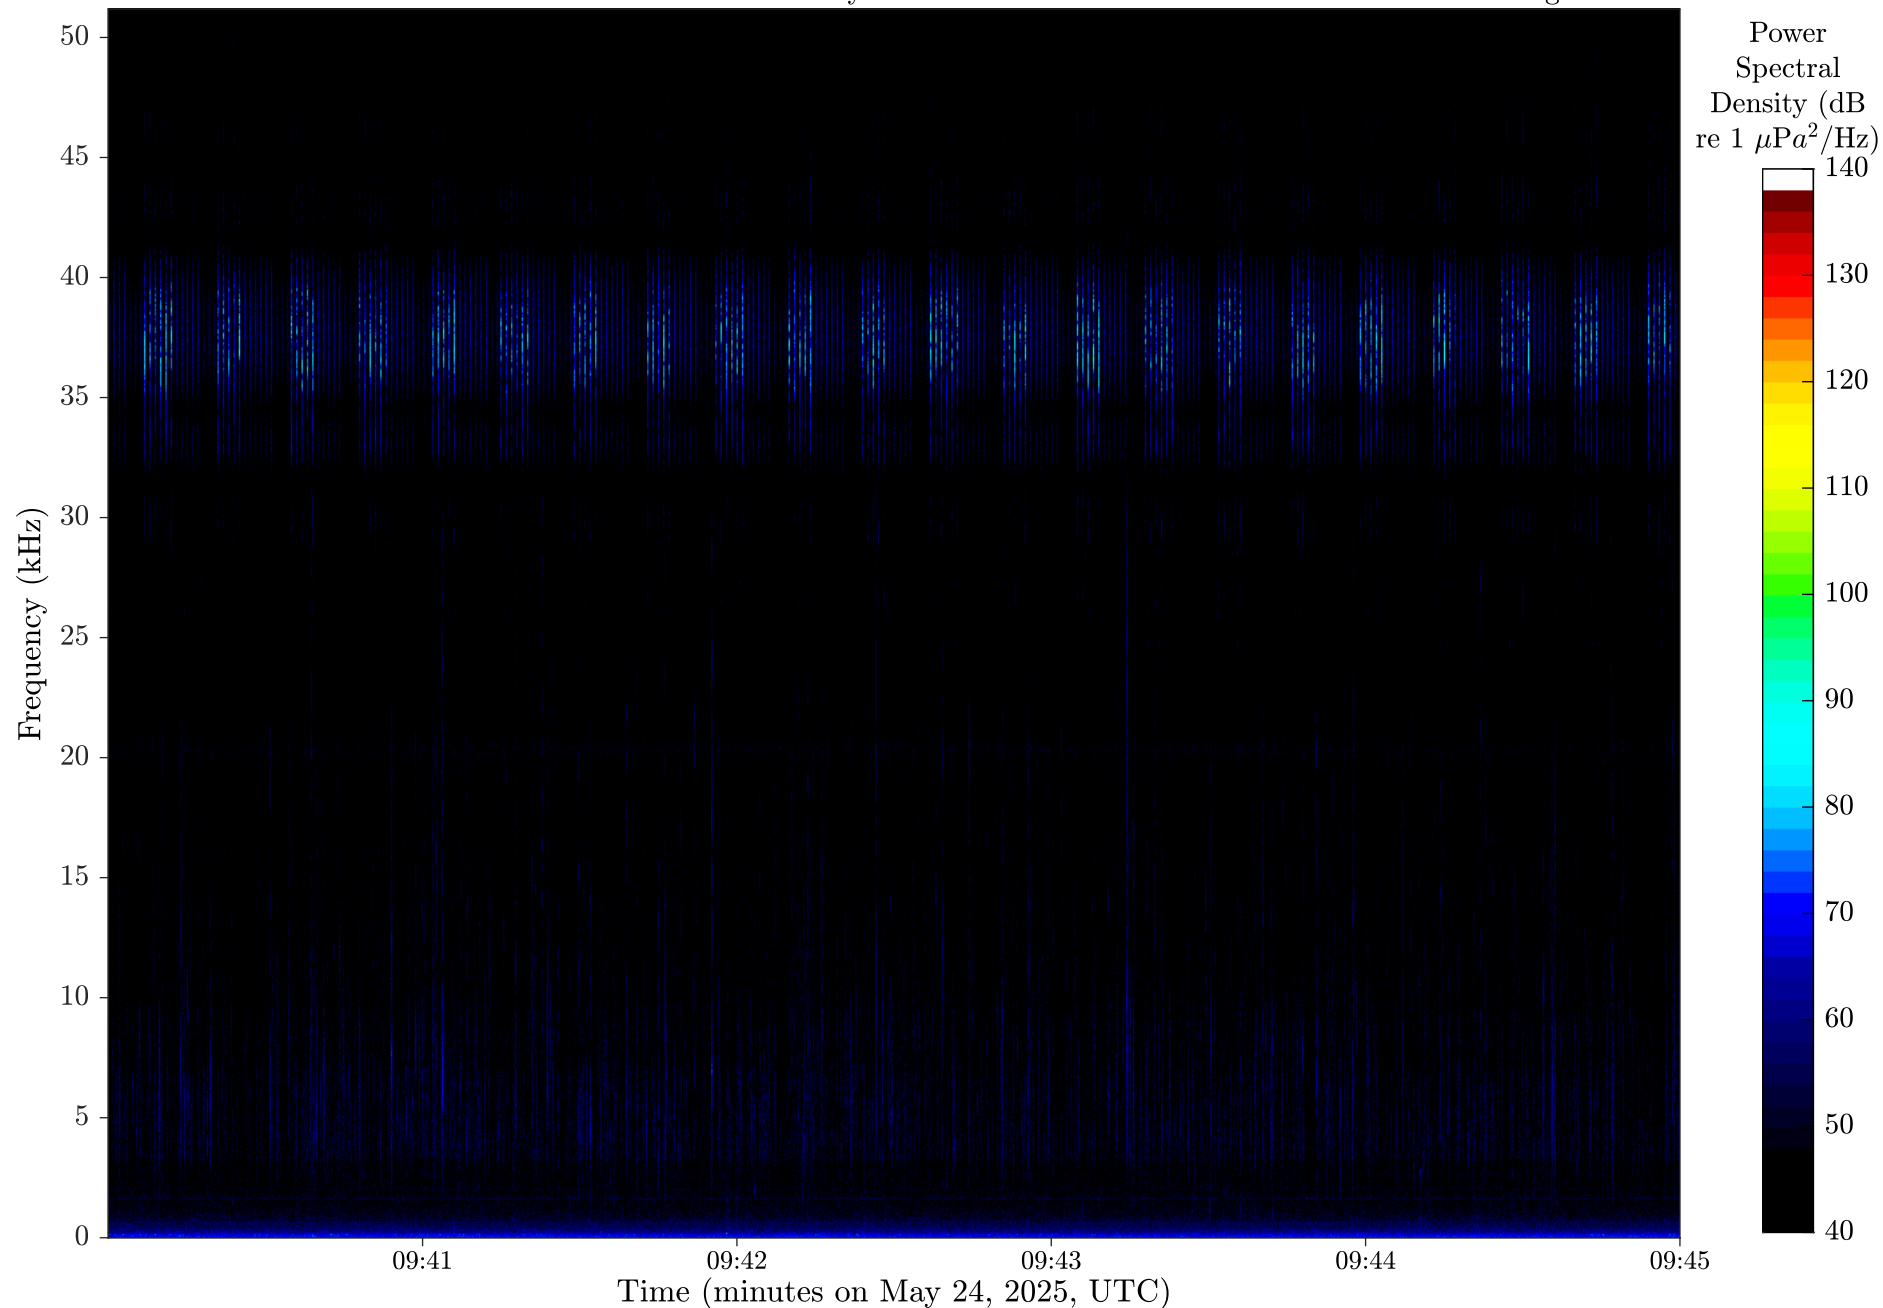


Comments: 36.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:10 UTC

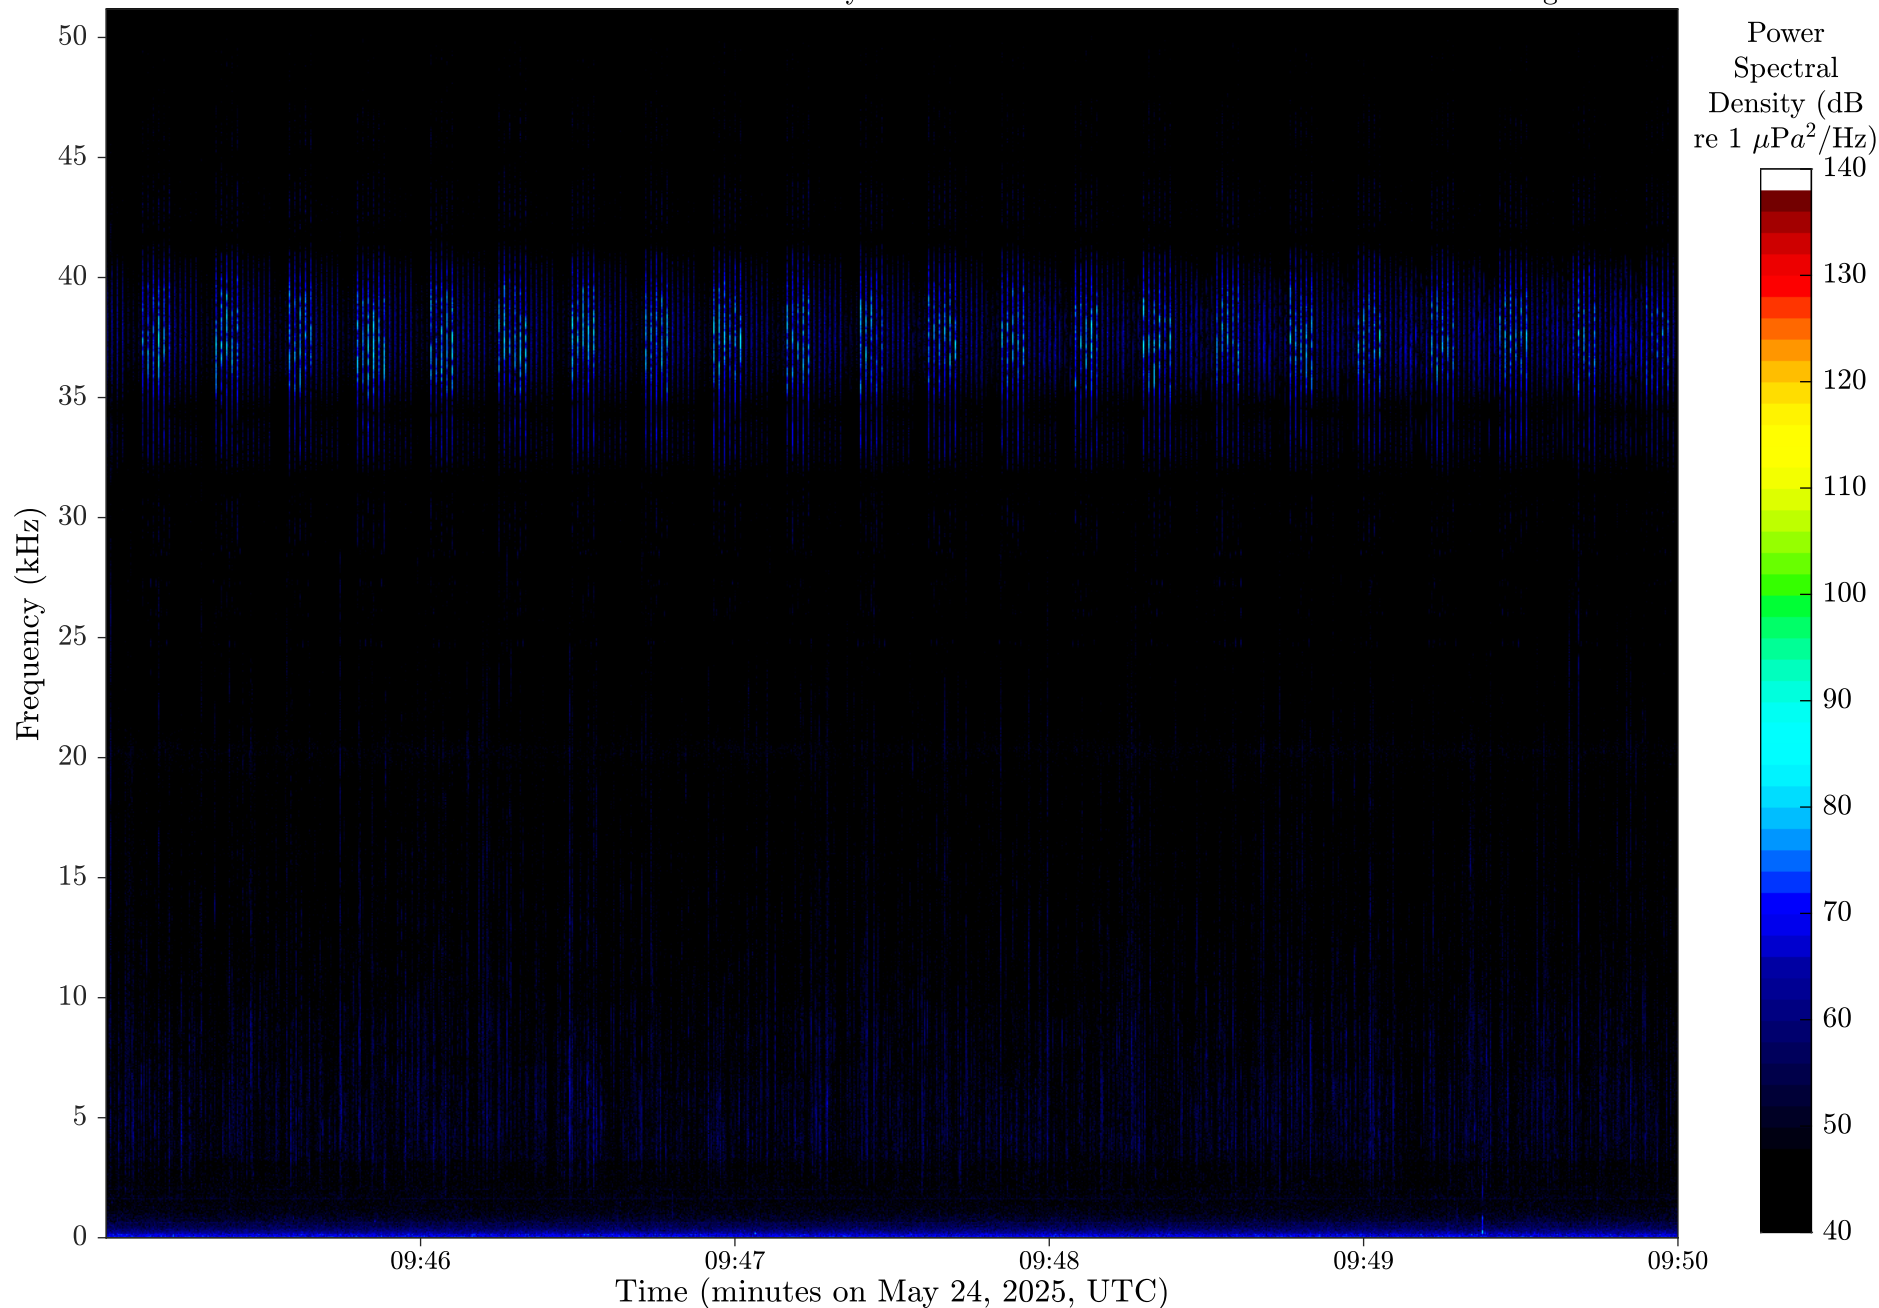


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:18 UTC

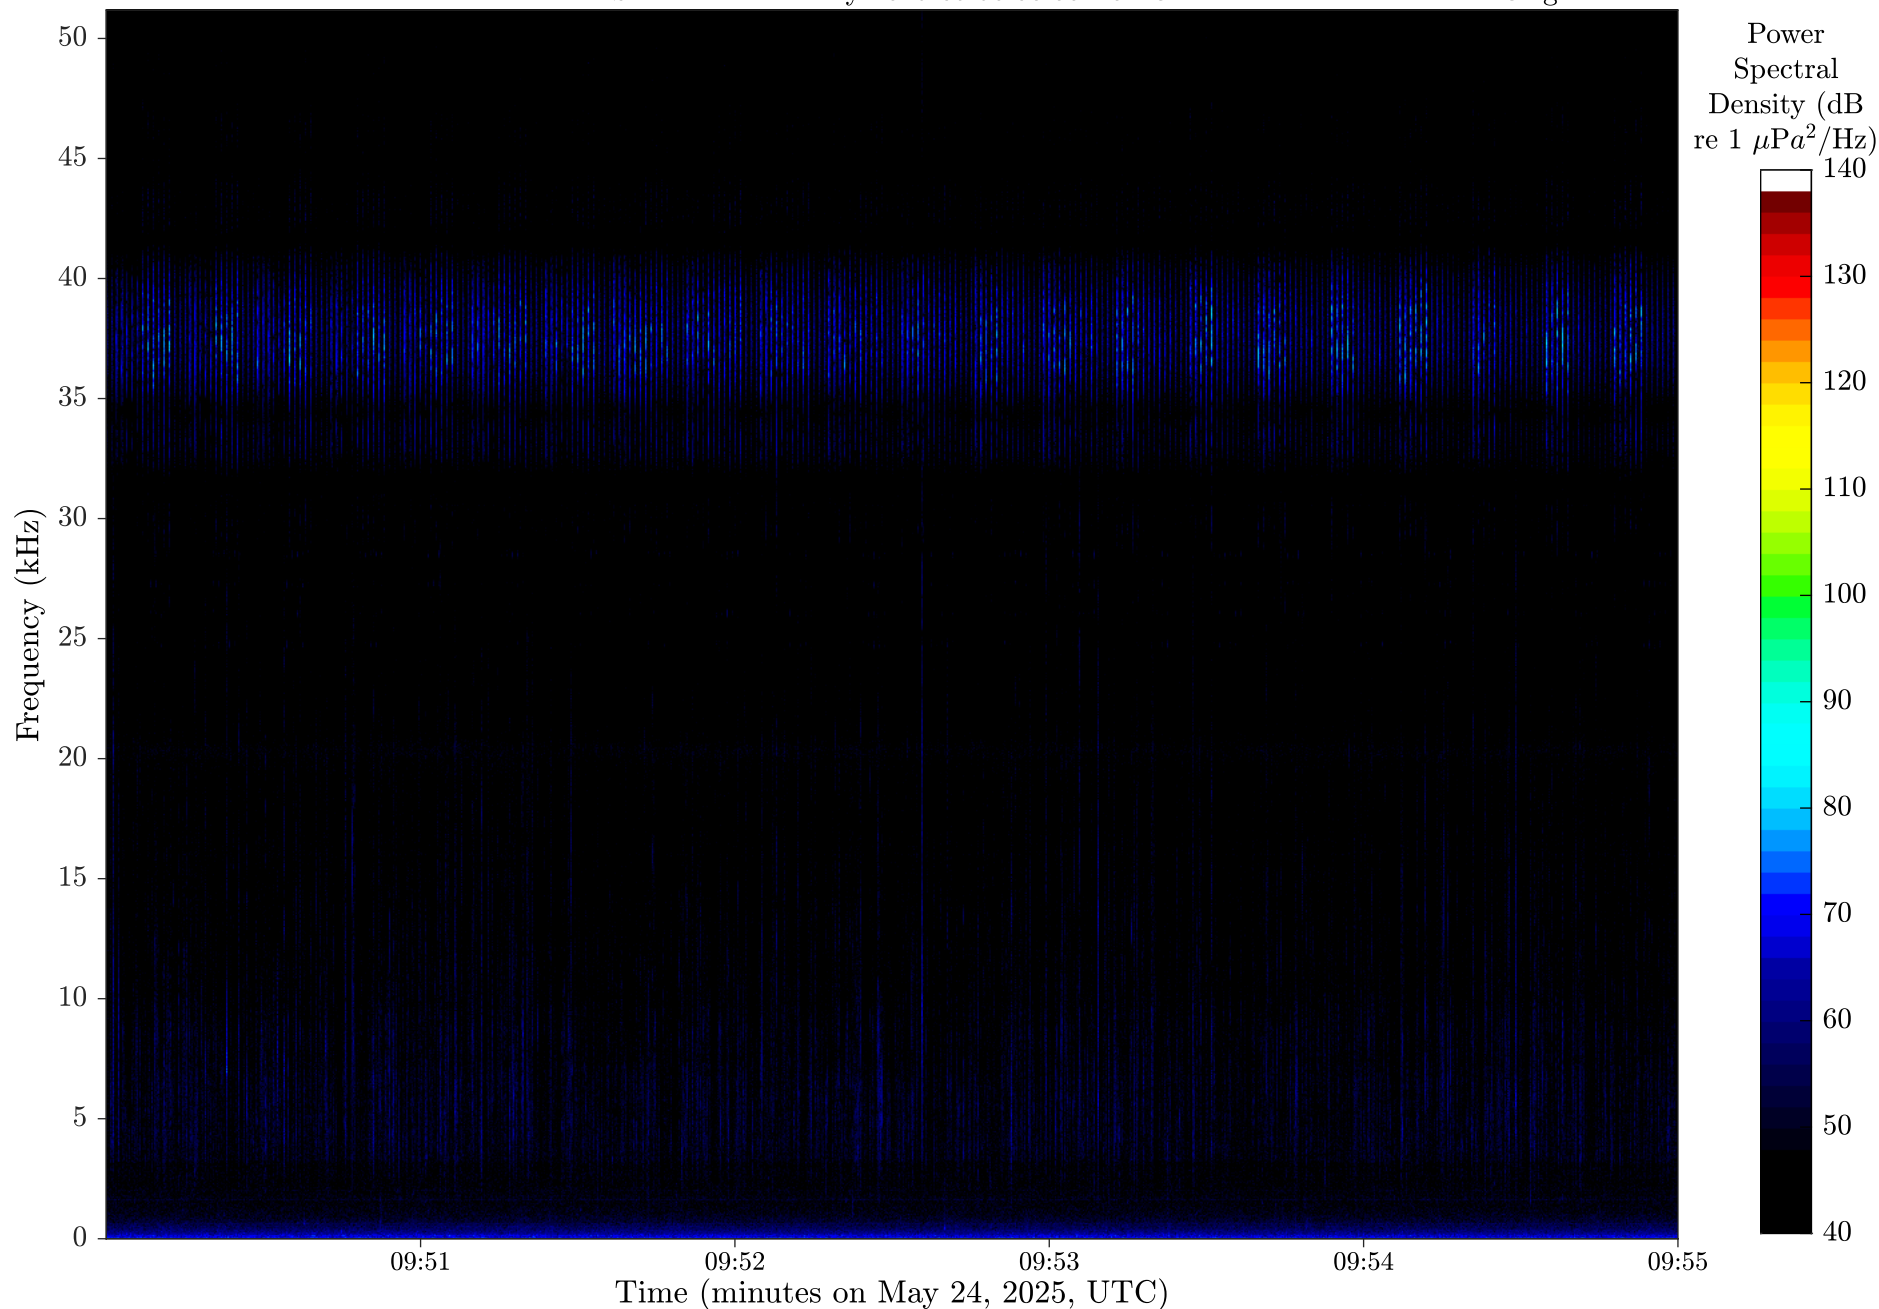


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:25 UTC

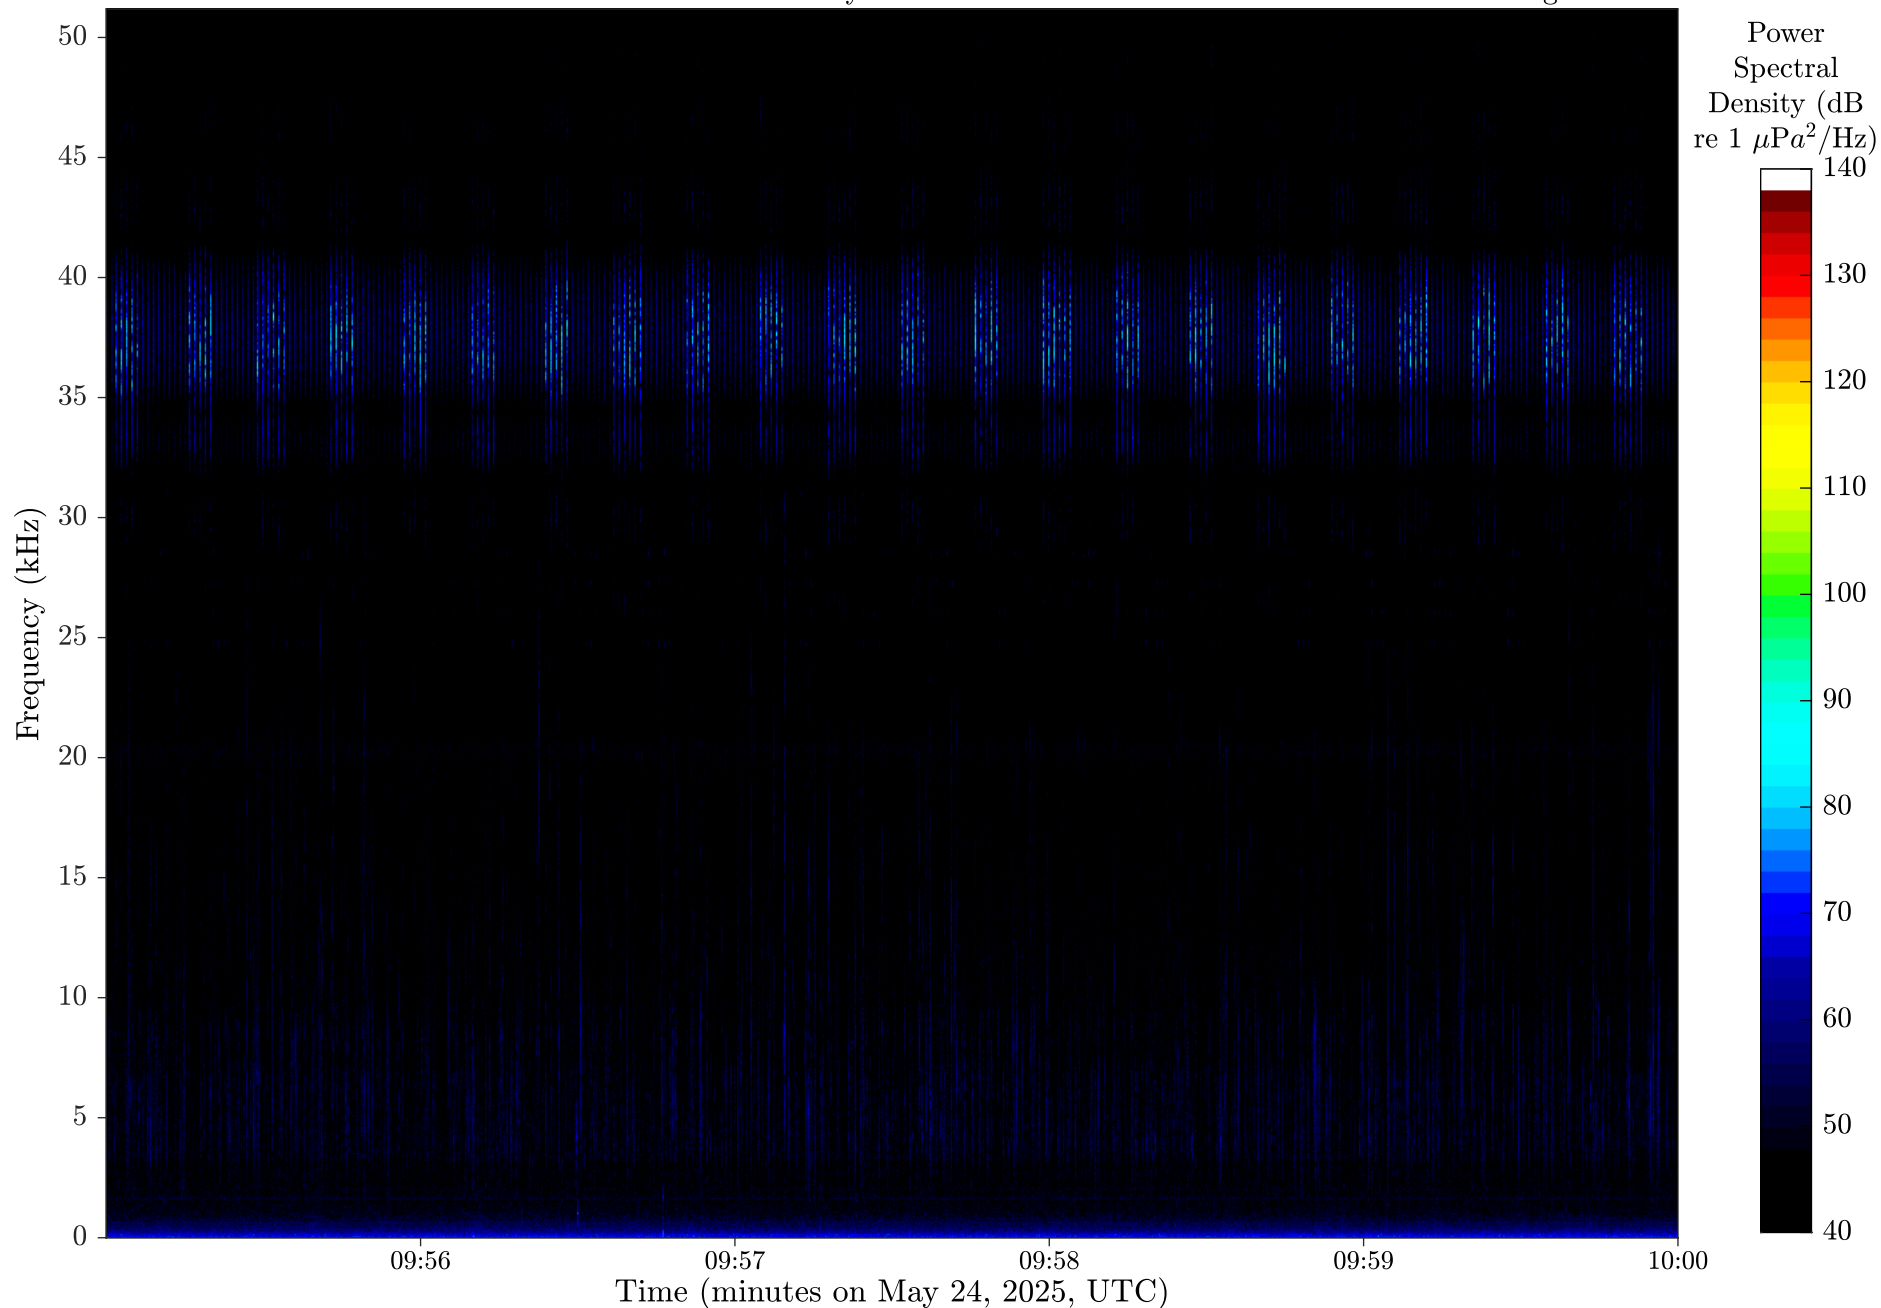


Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:35:33 UTC

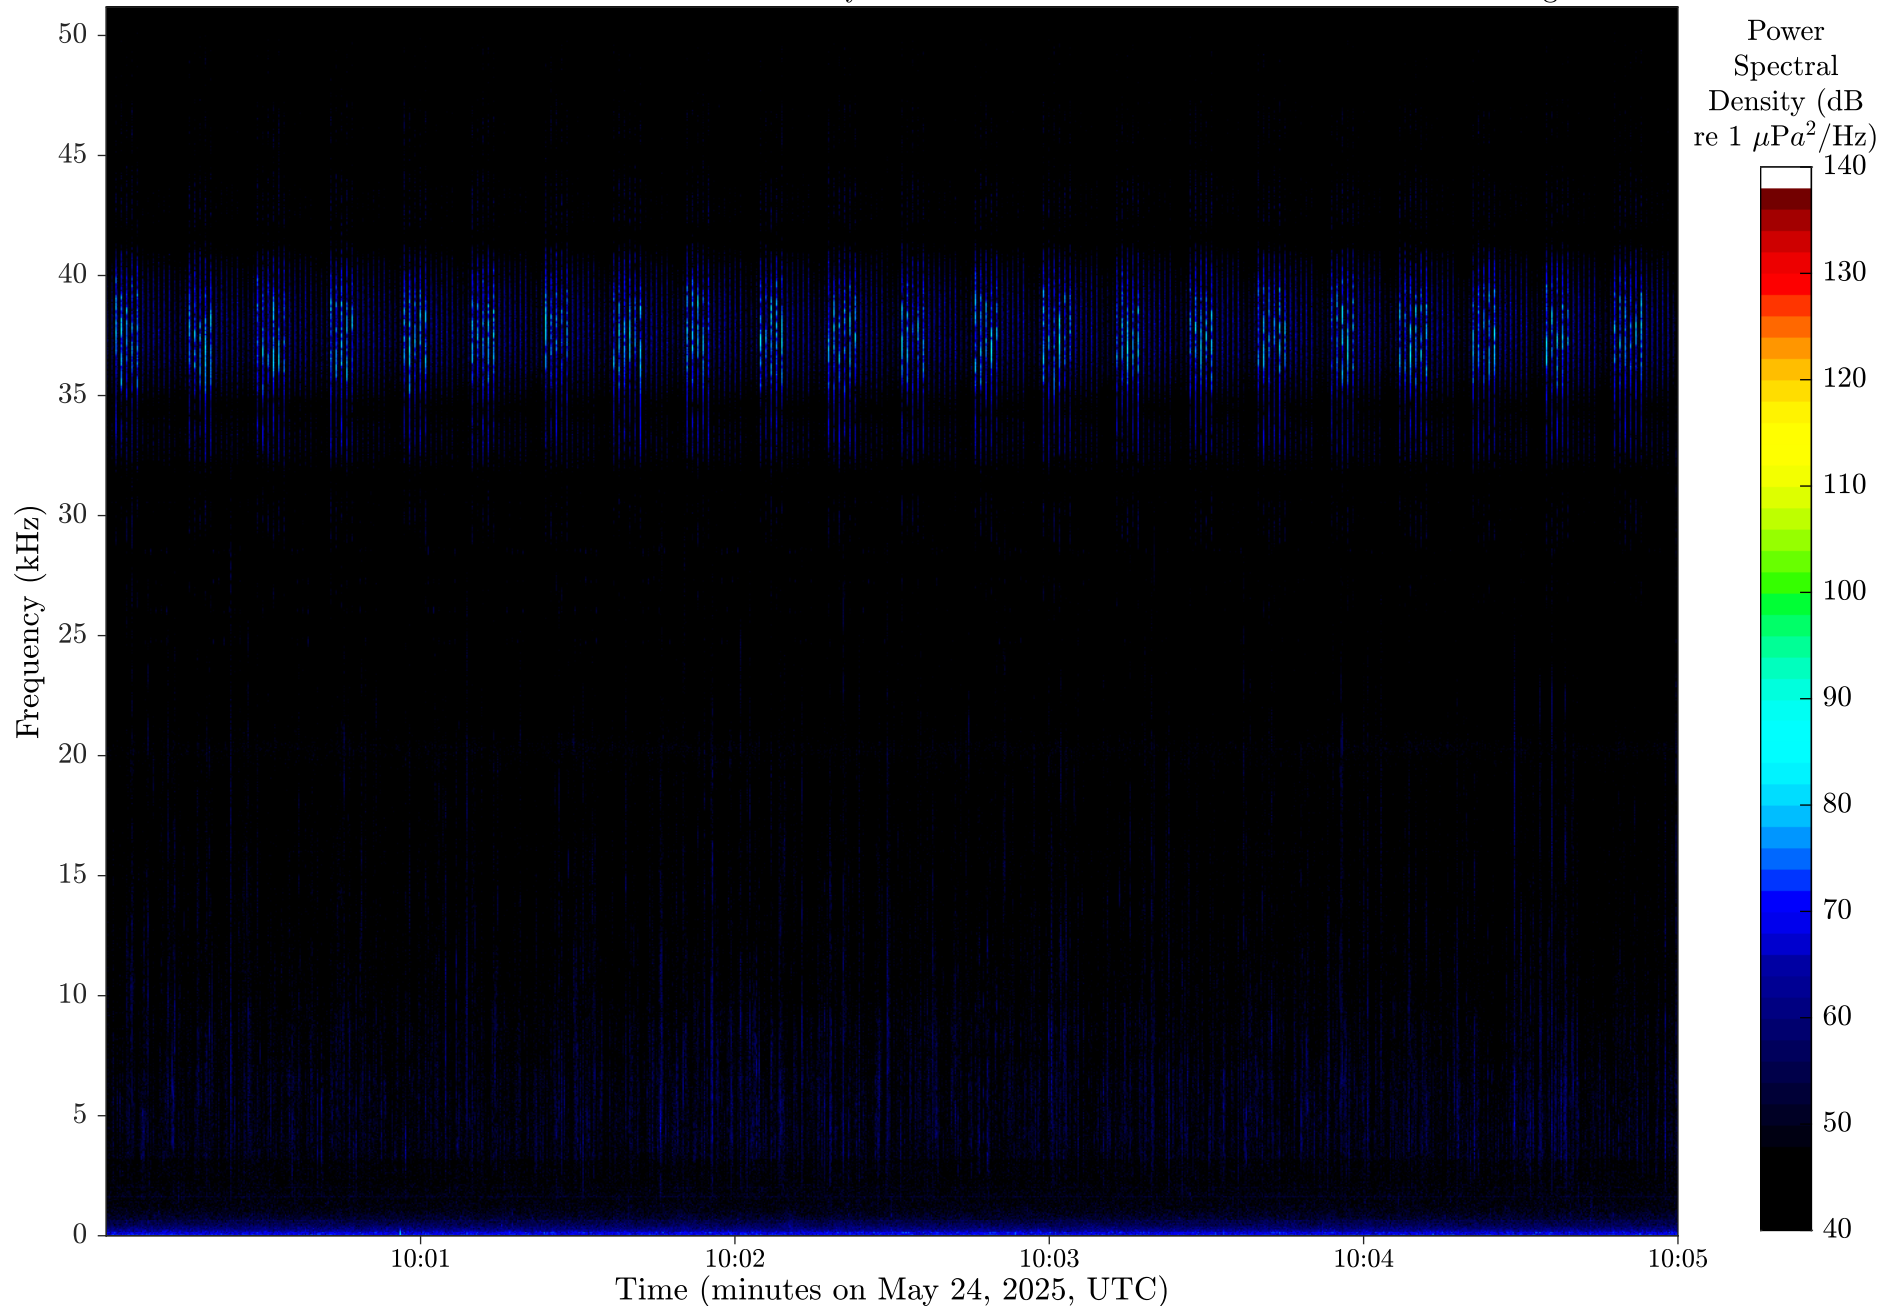


Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:35:41 UTC

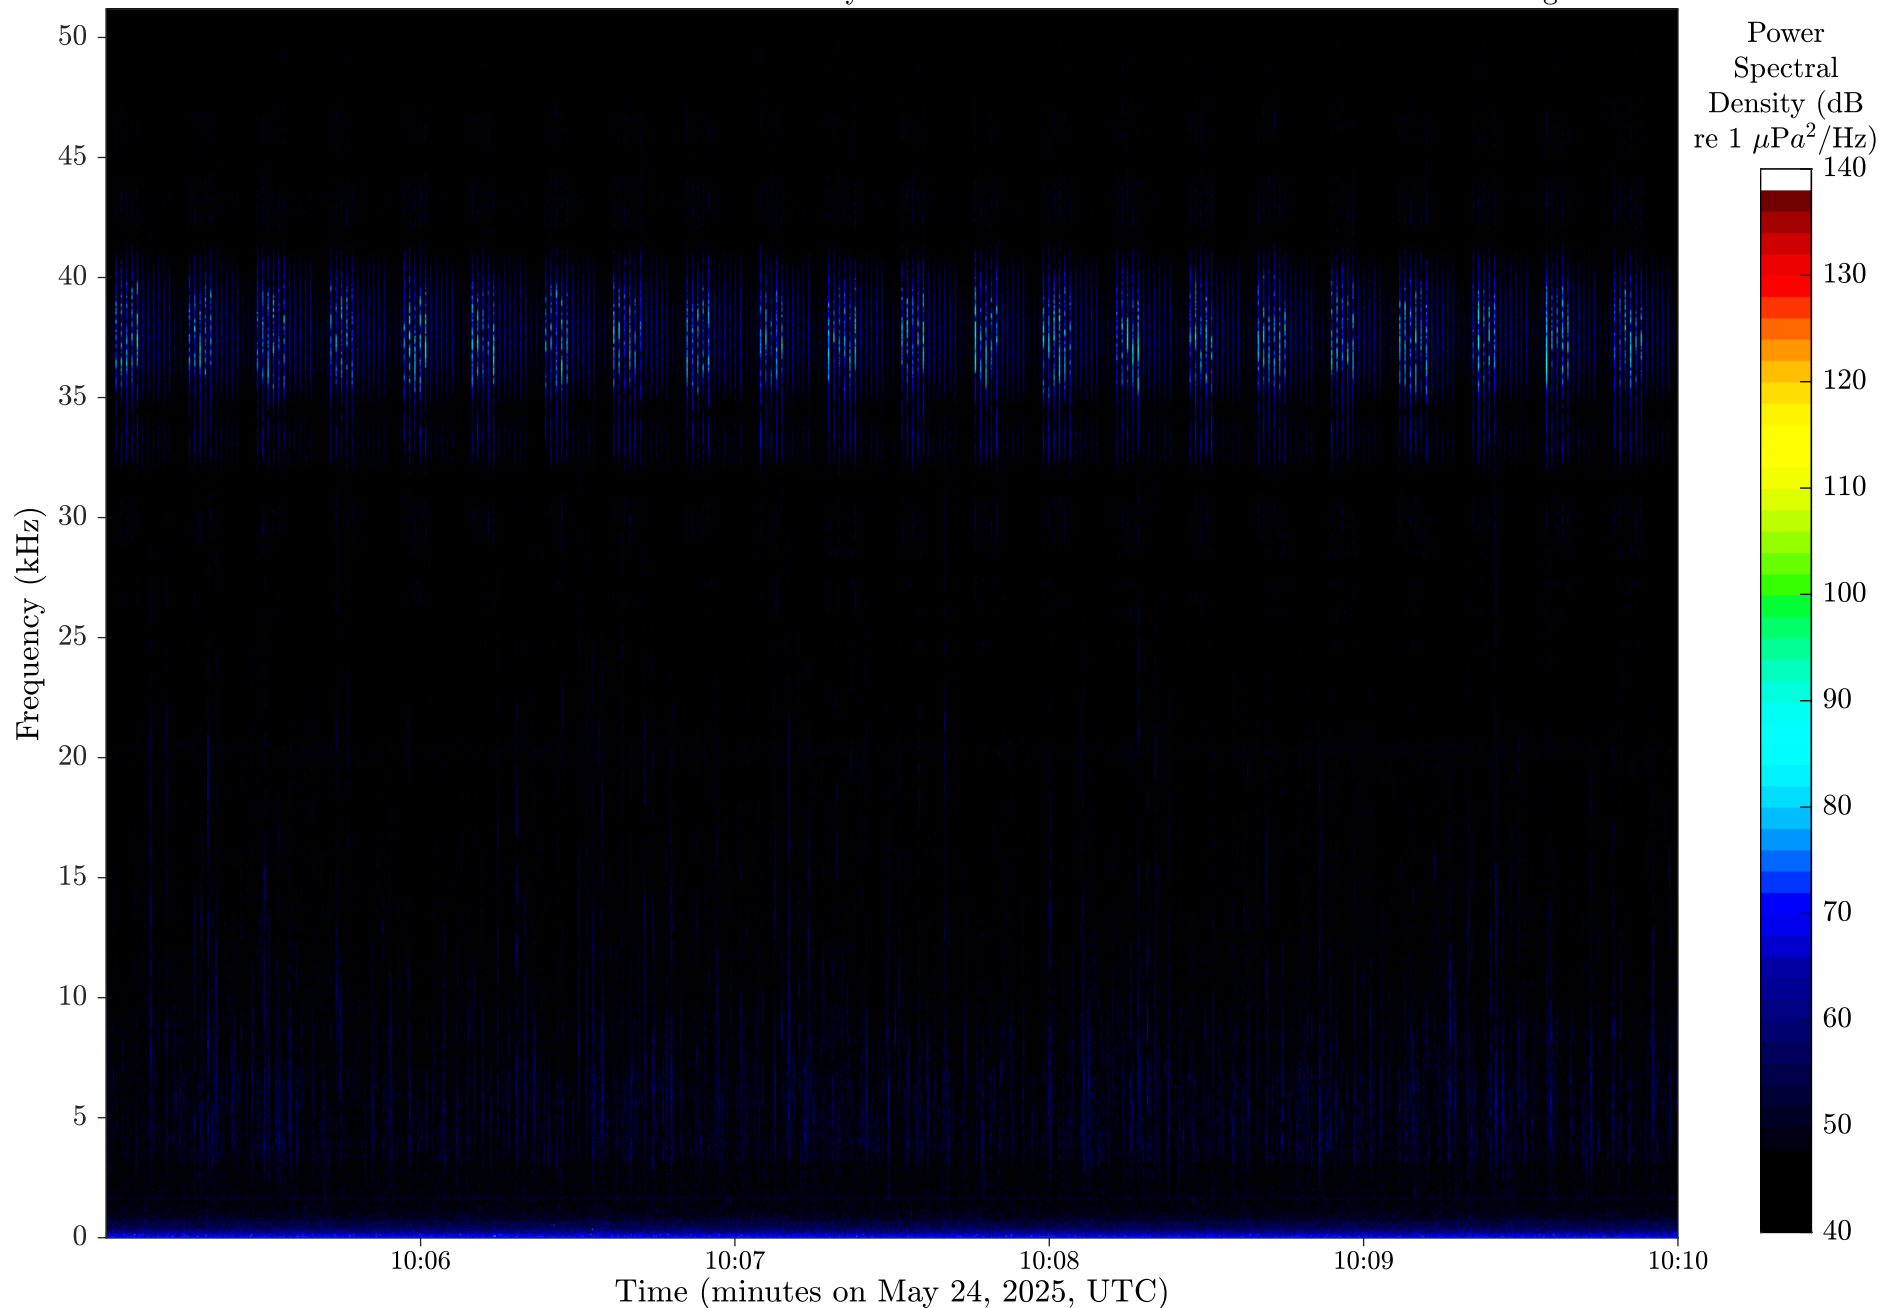


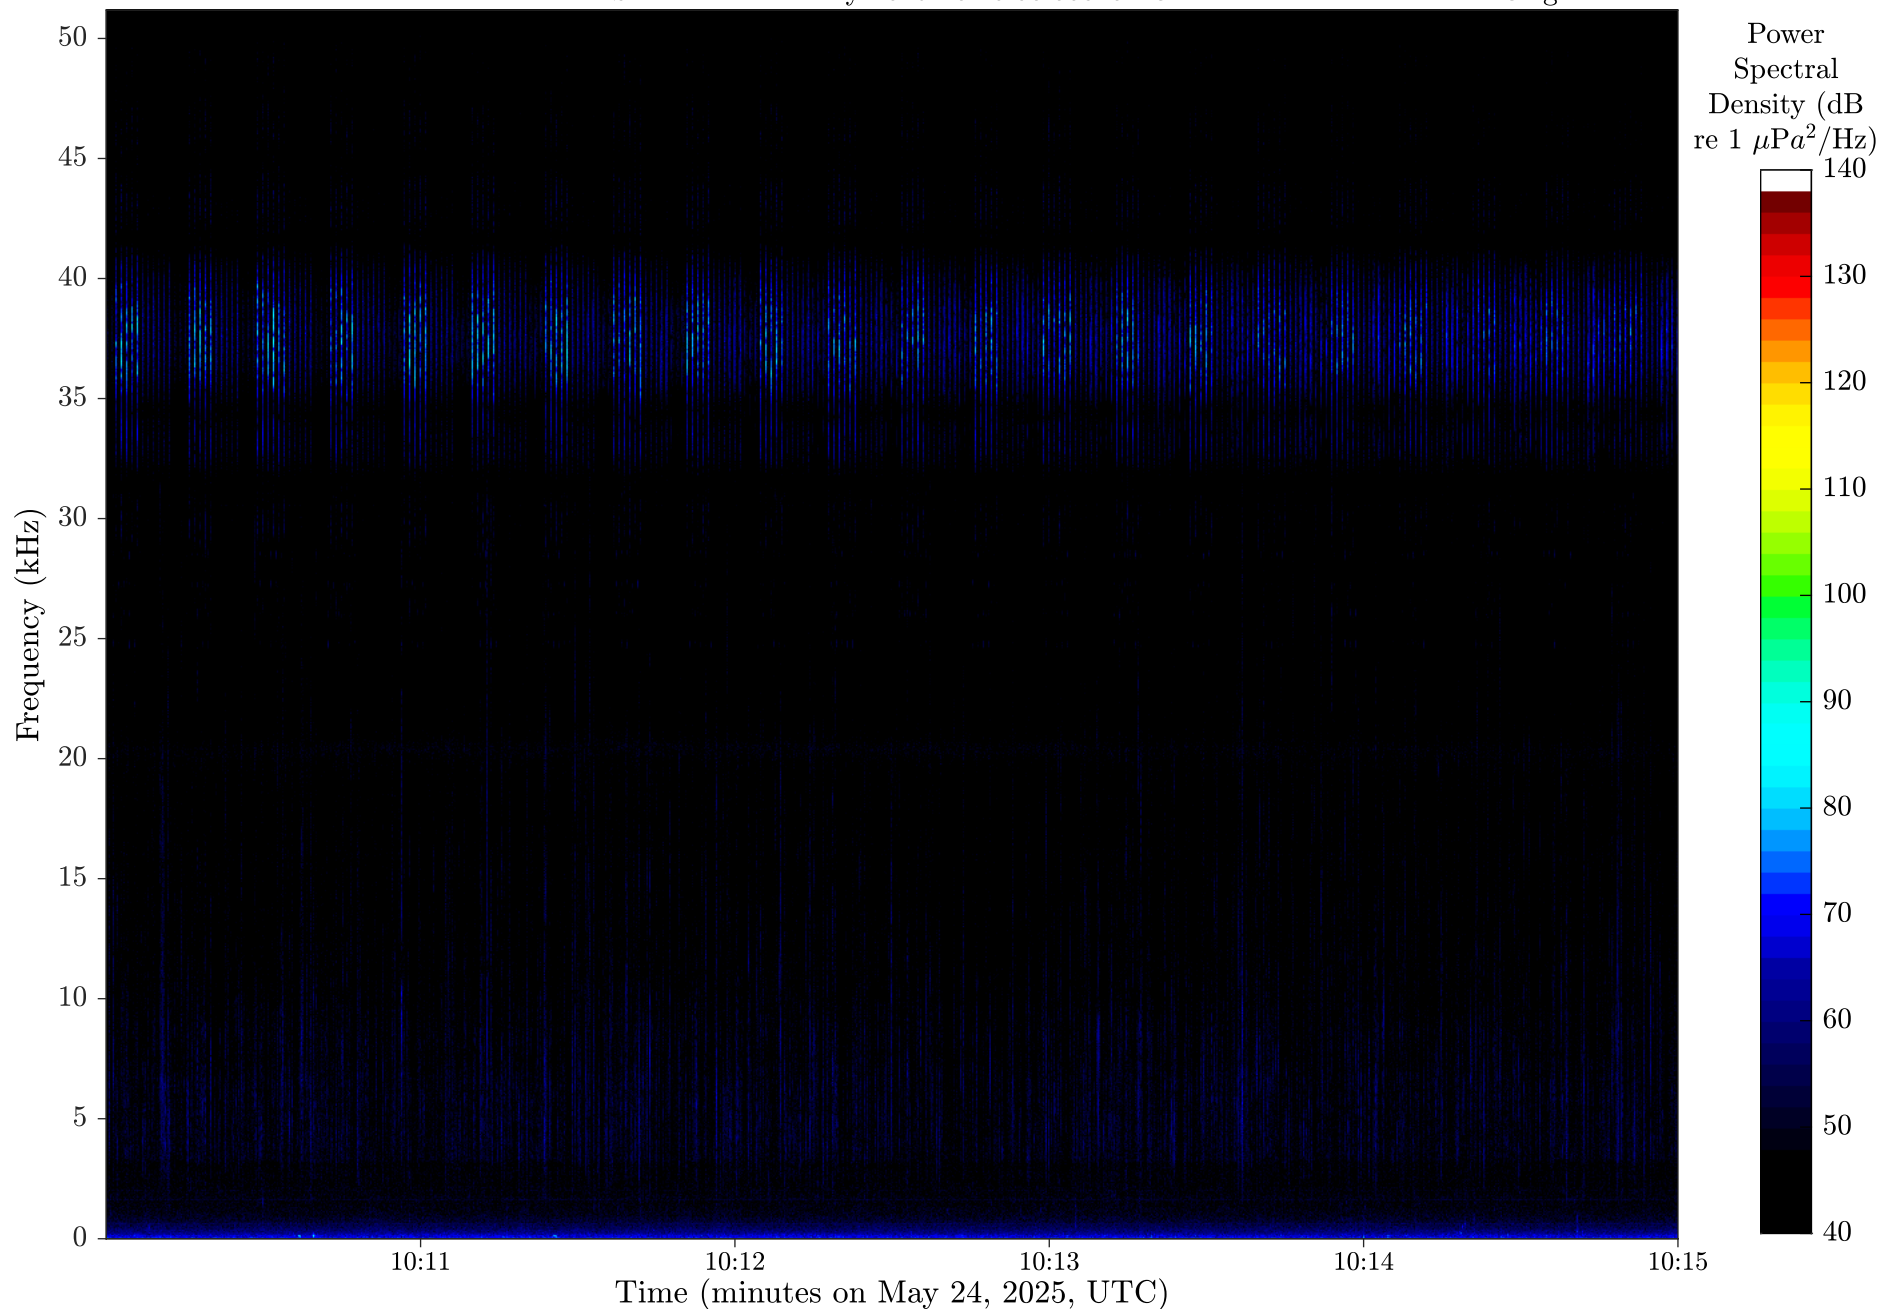

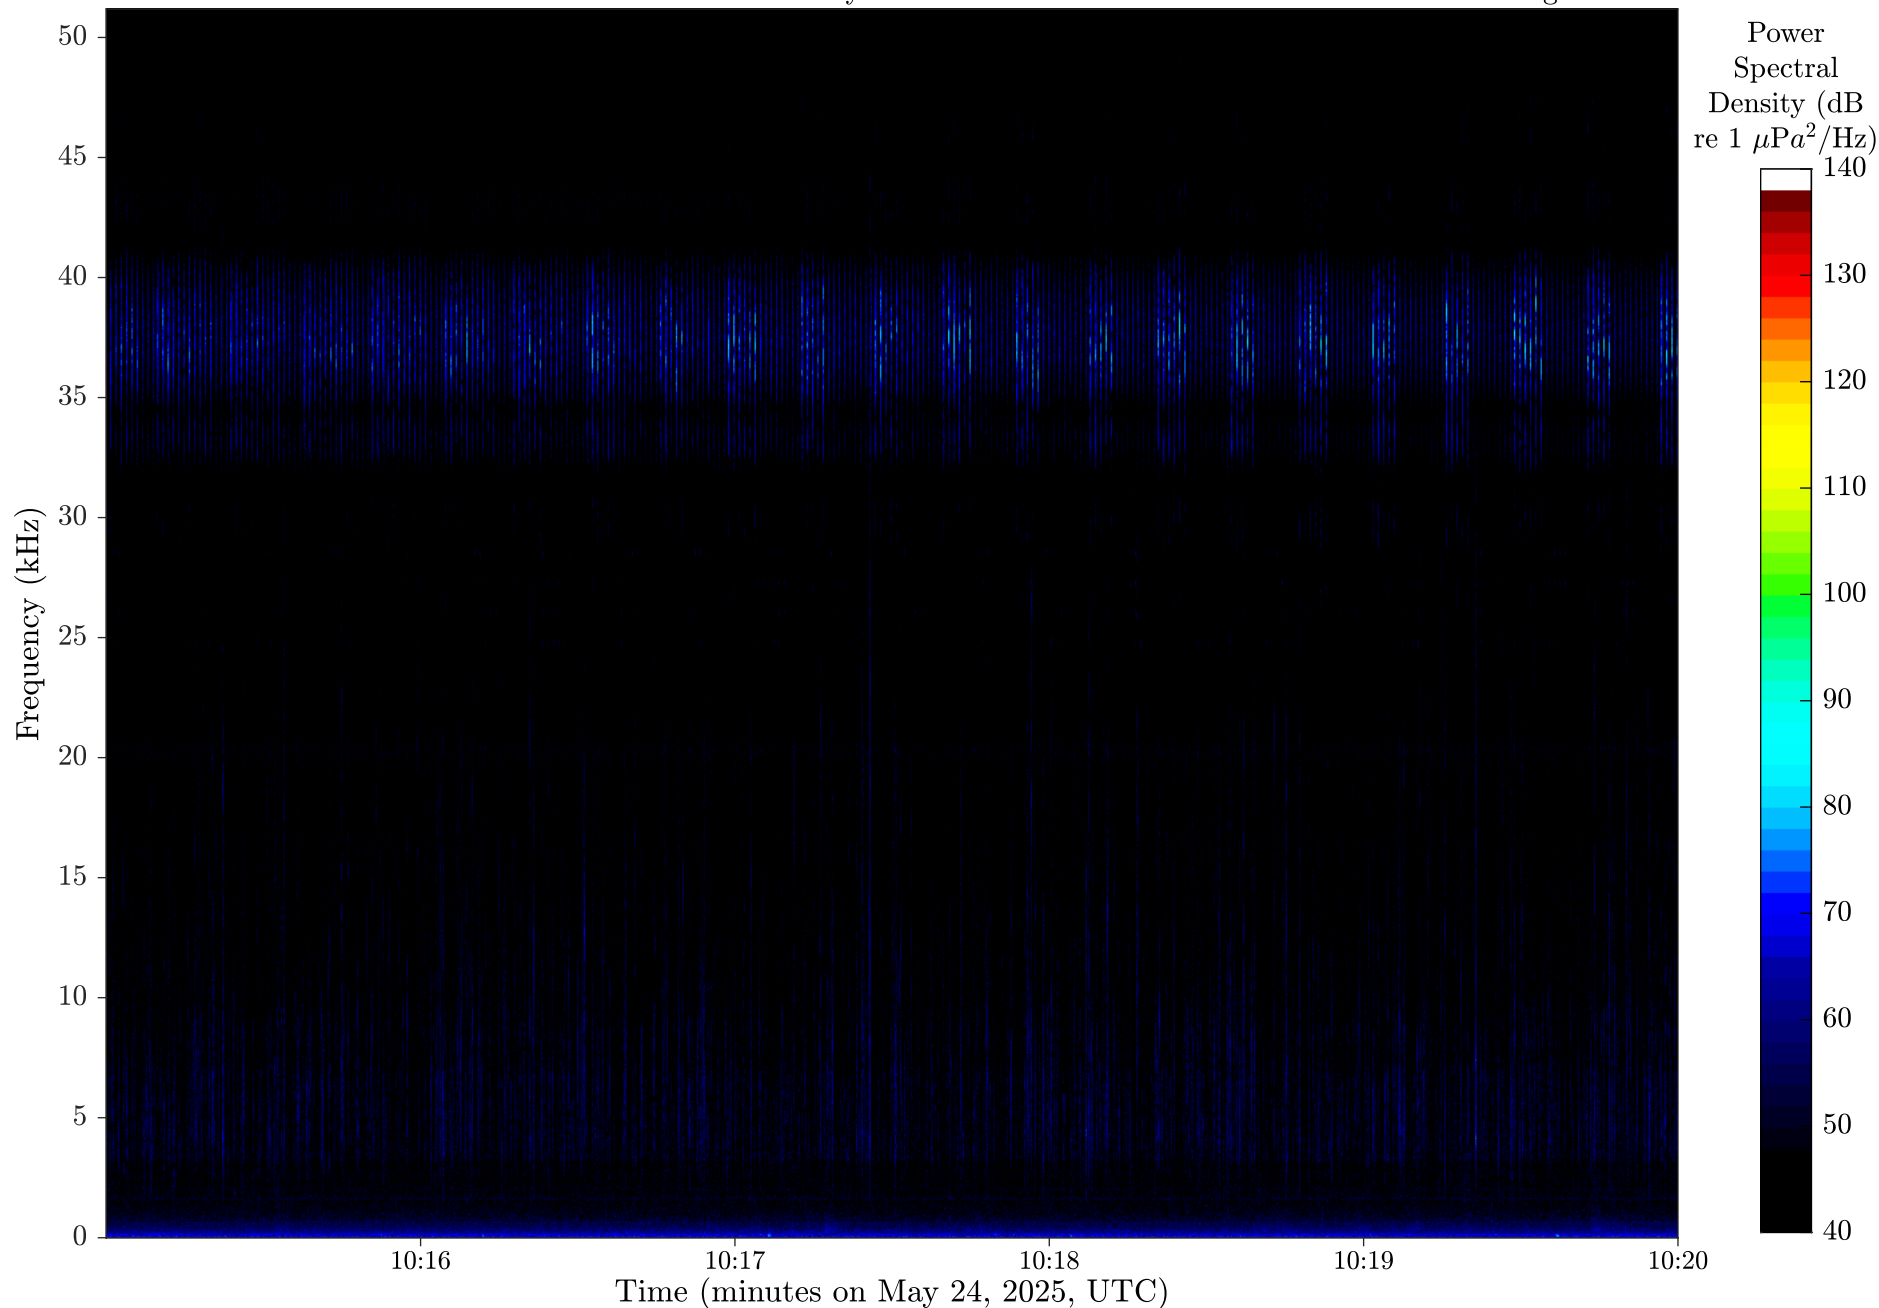


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:04 UTC

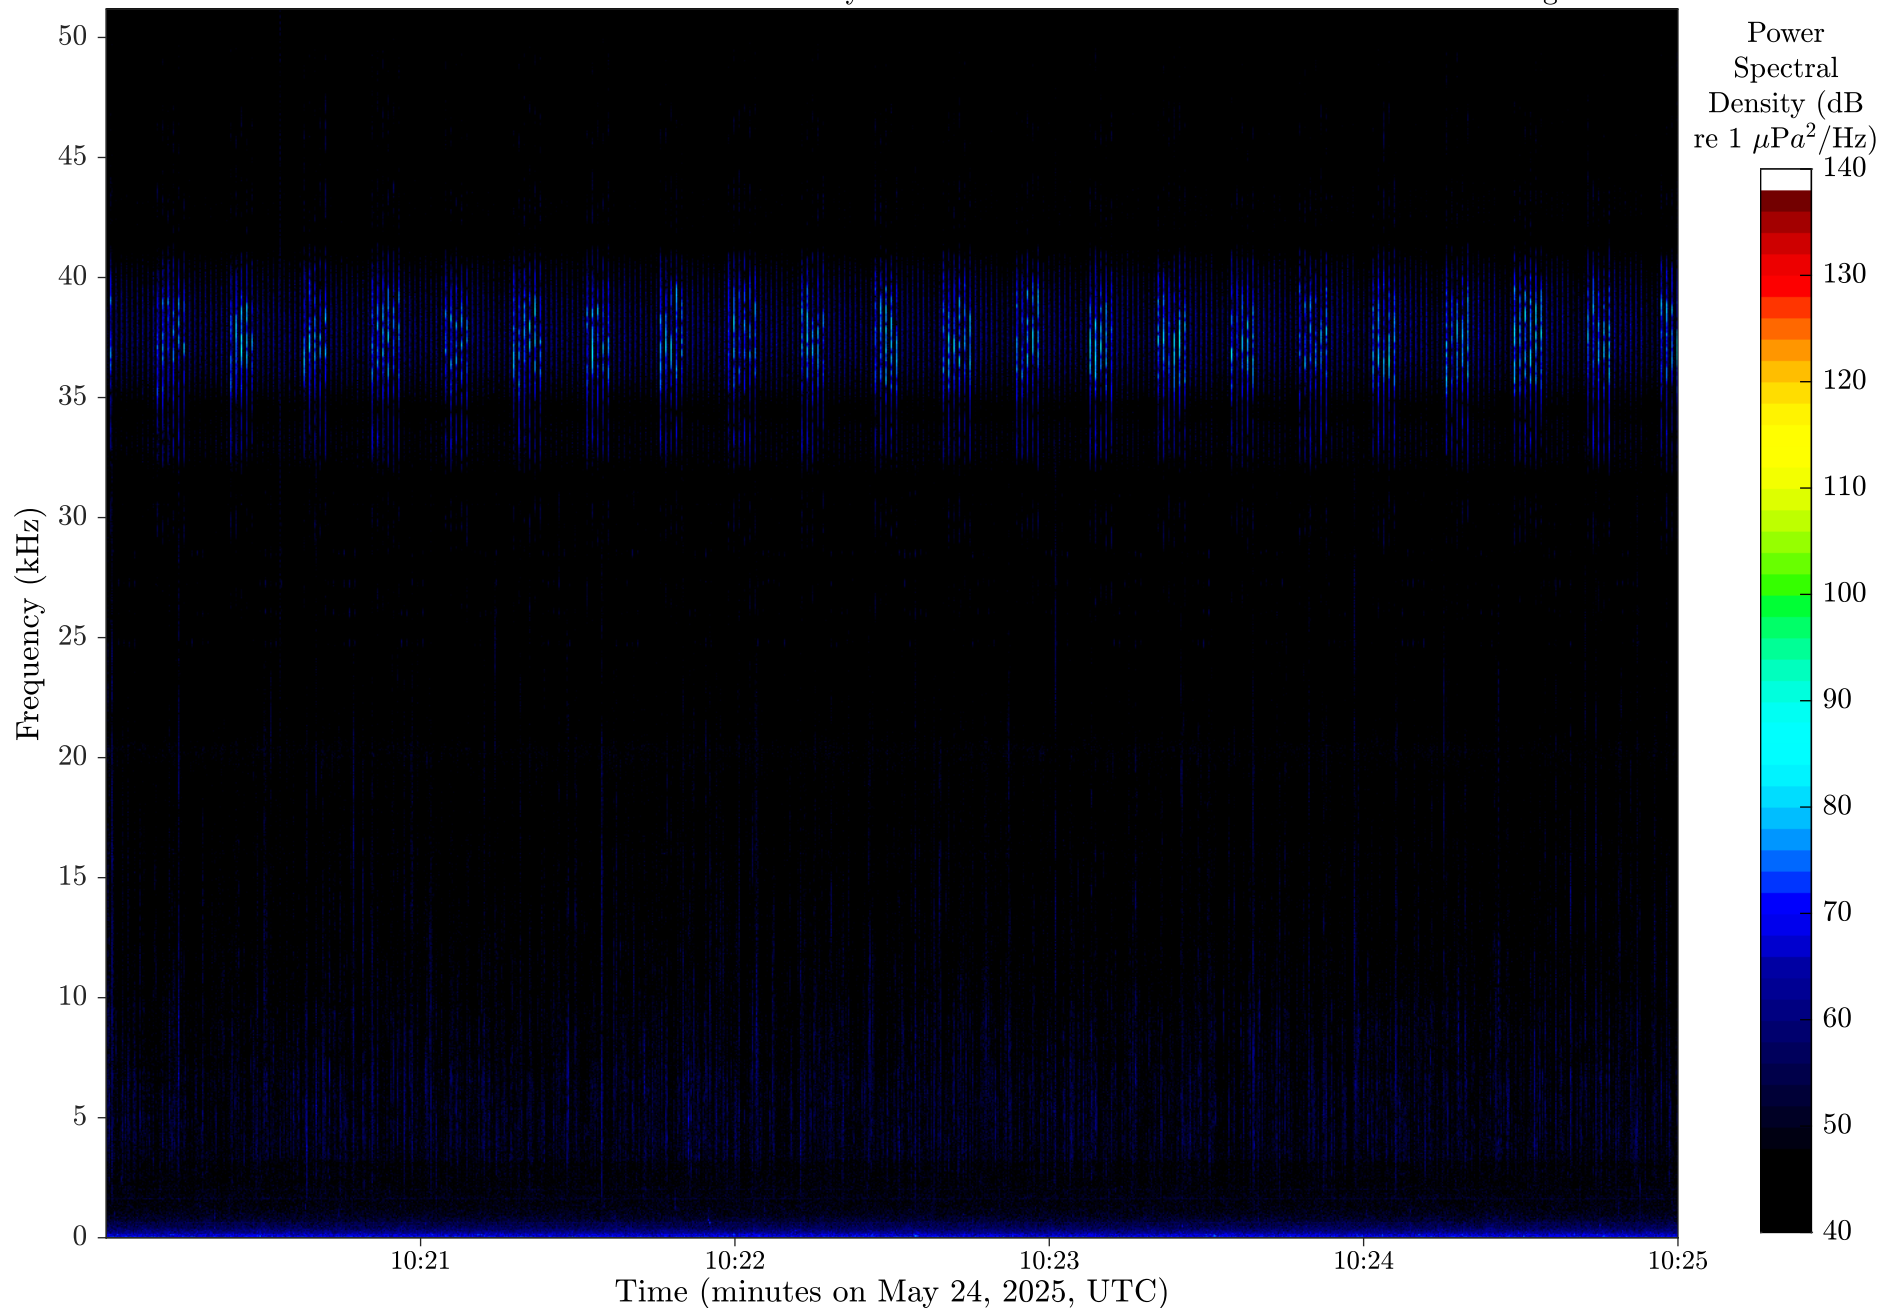


Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:36:12 UTC

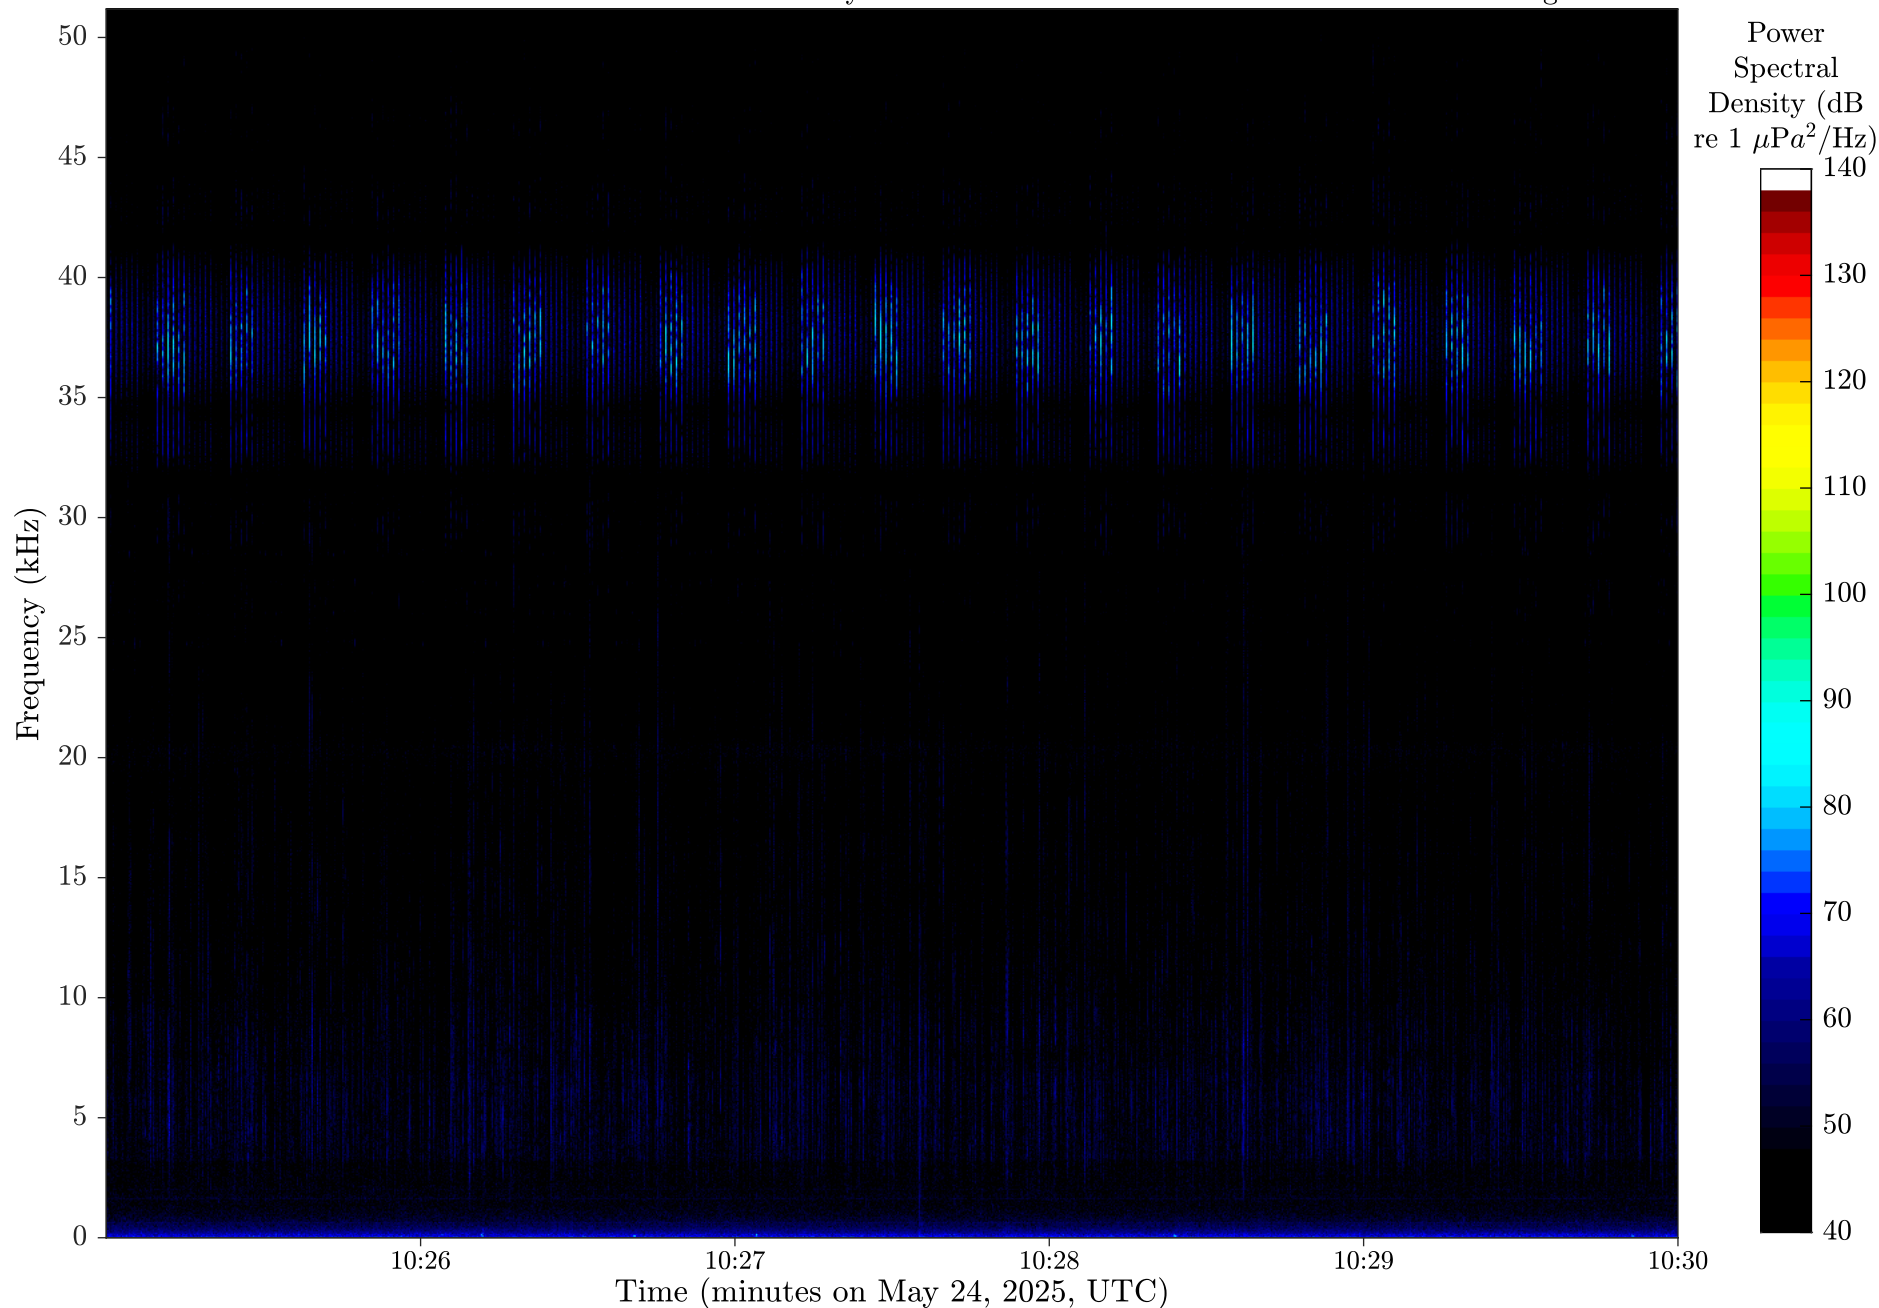

Comments: 35.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:36:20 UTC

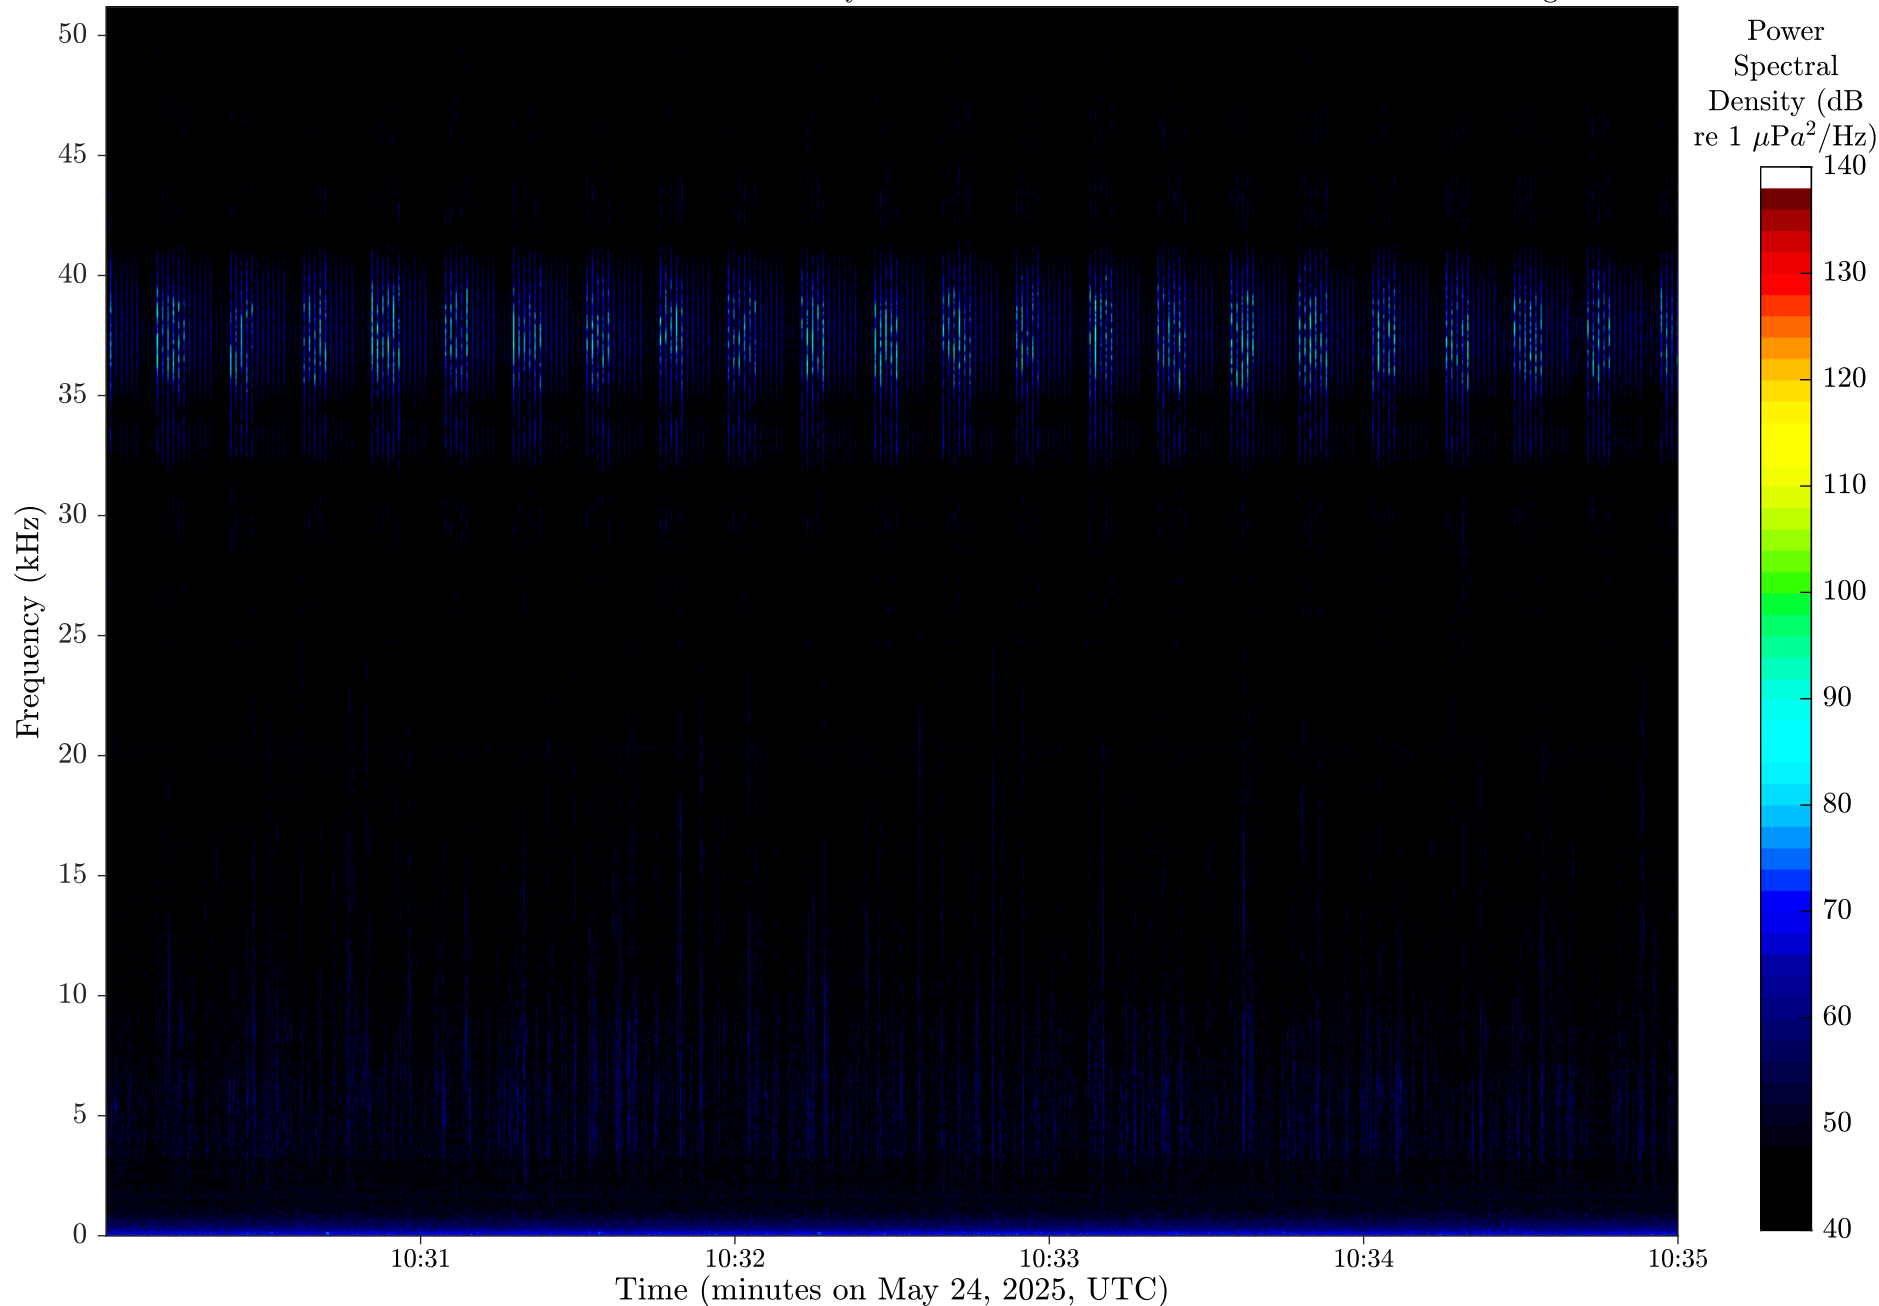


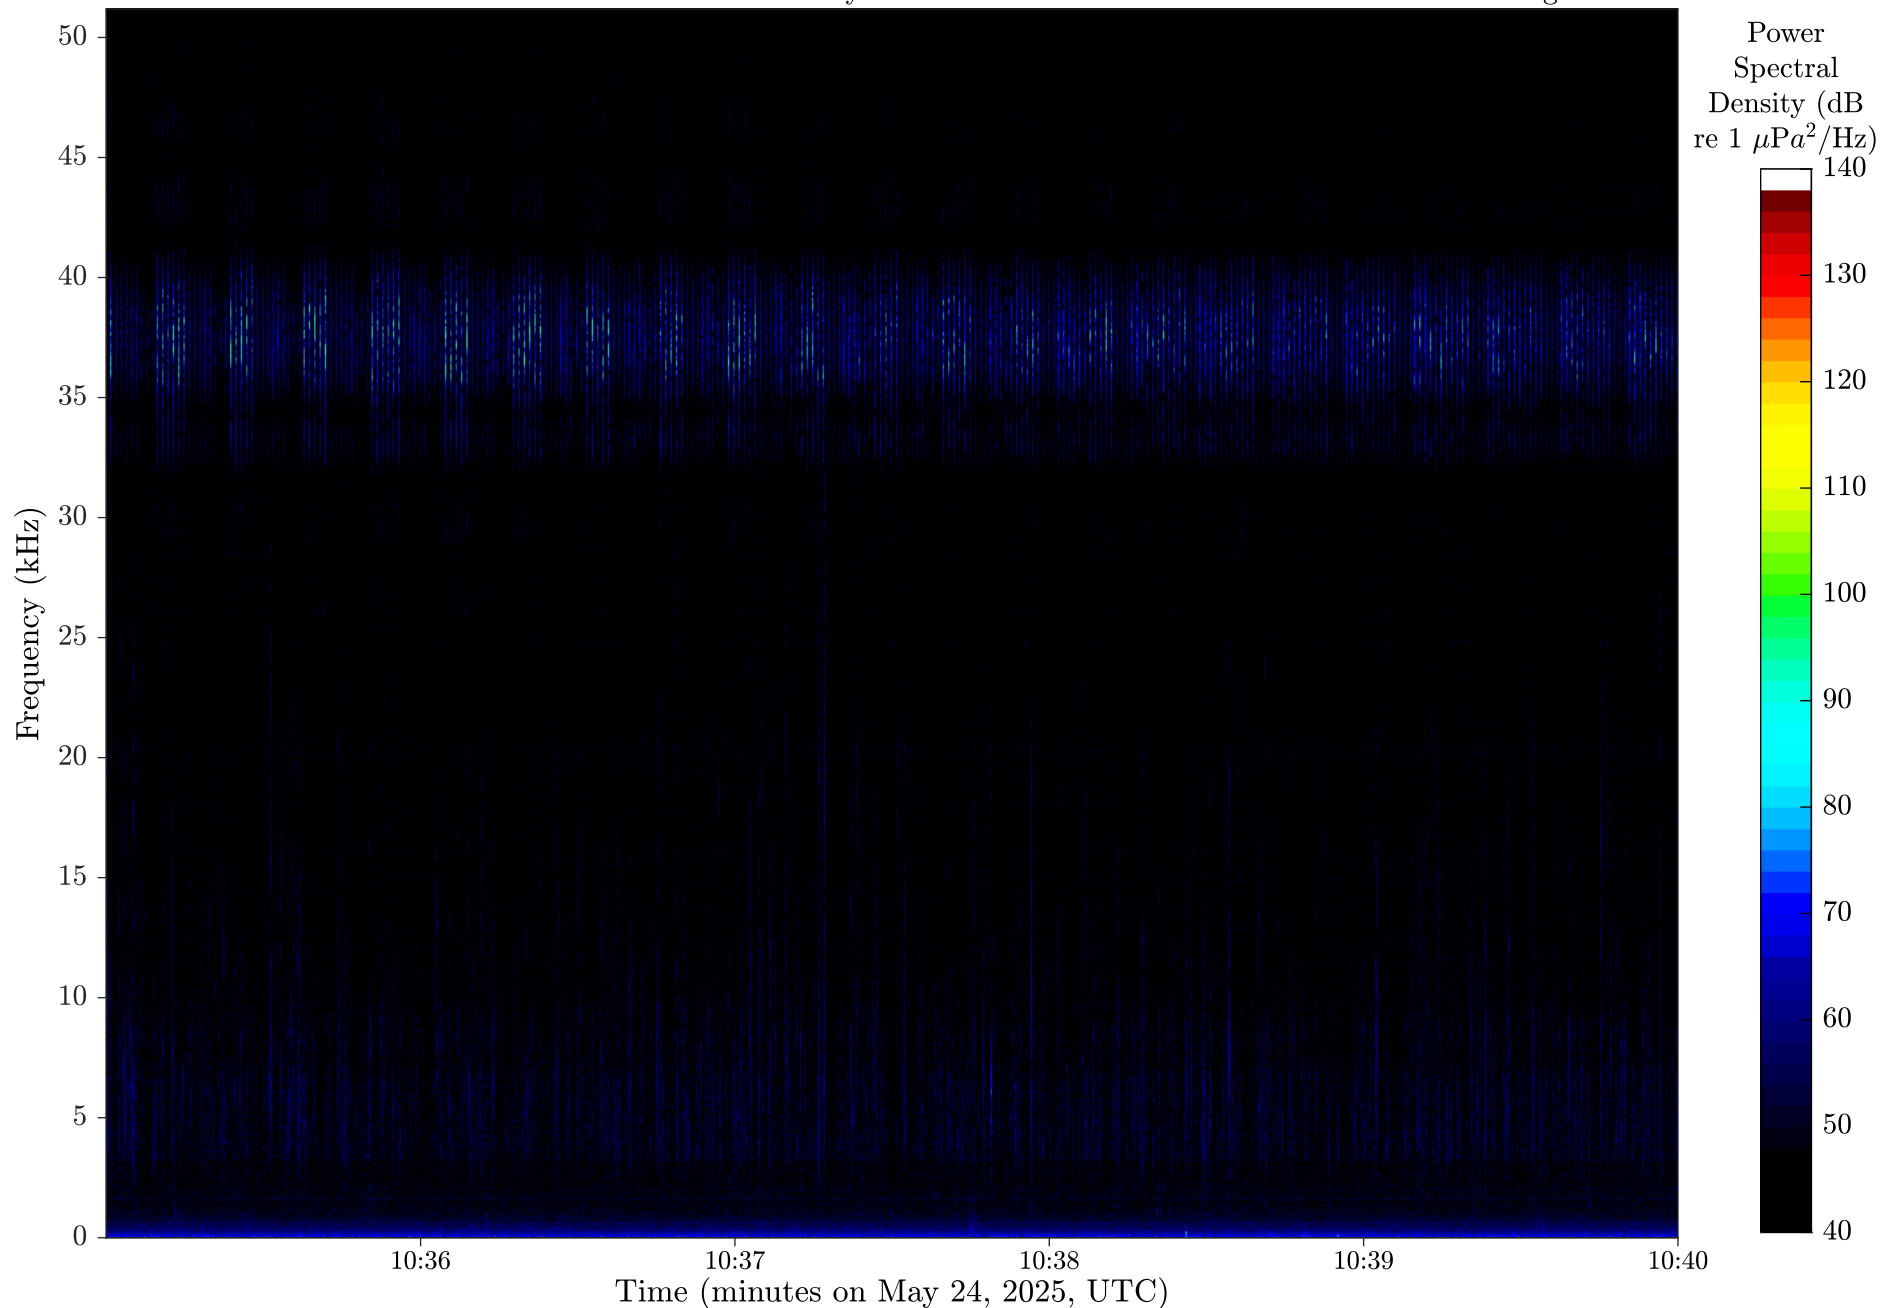

Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:36:35 UTC

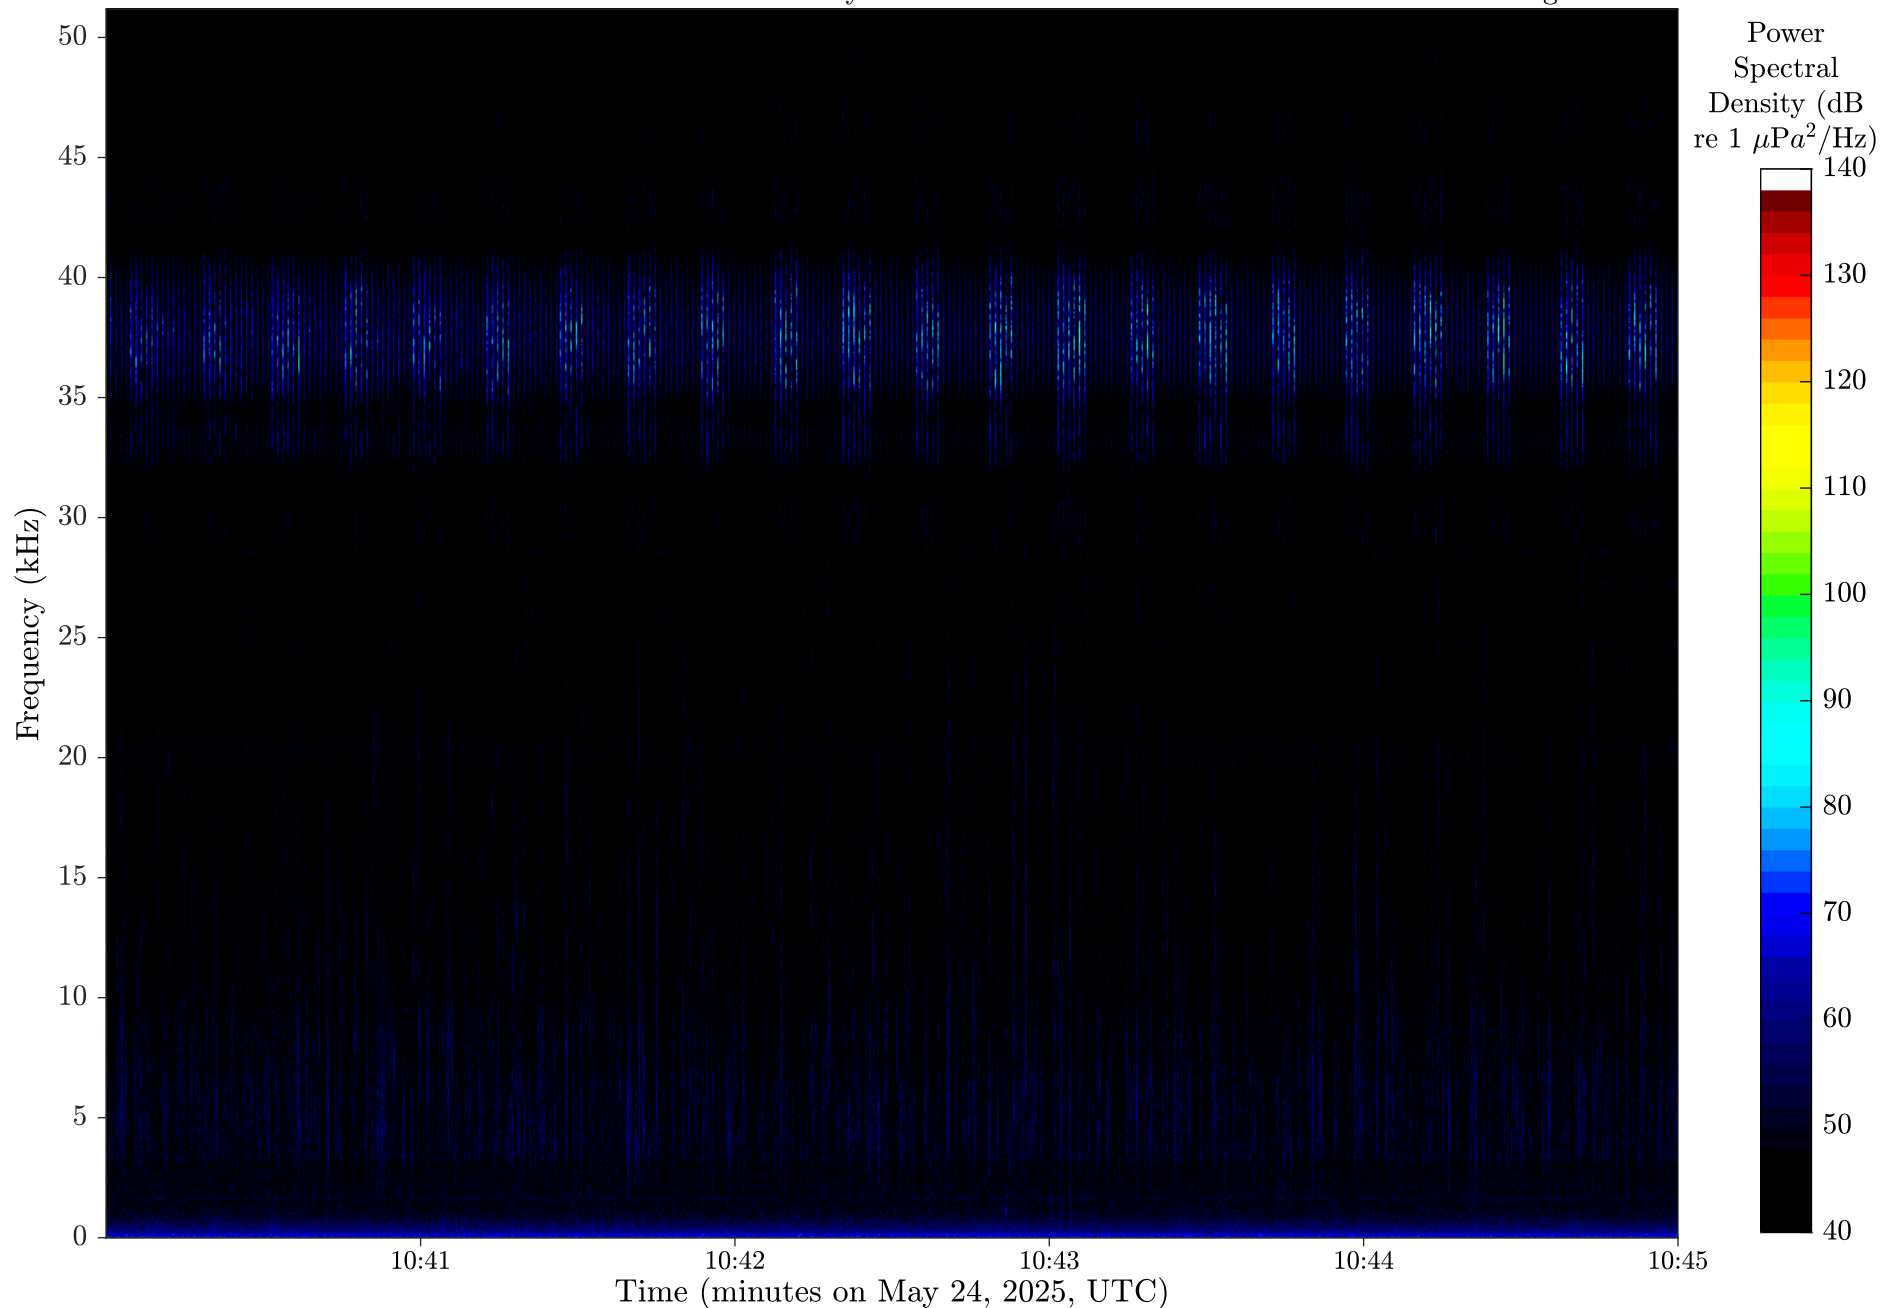

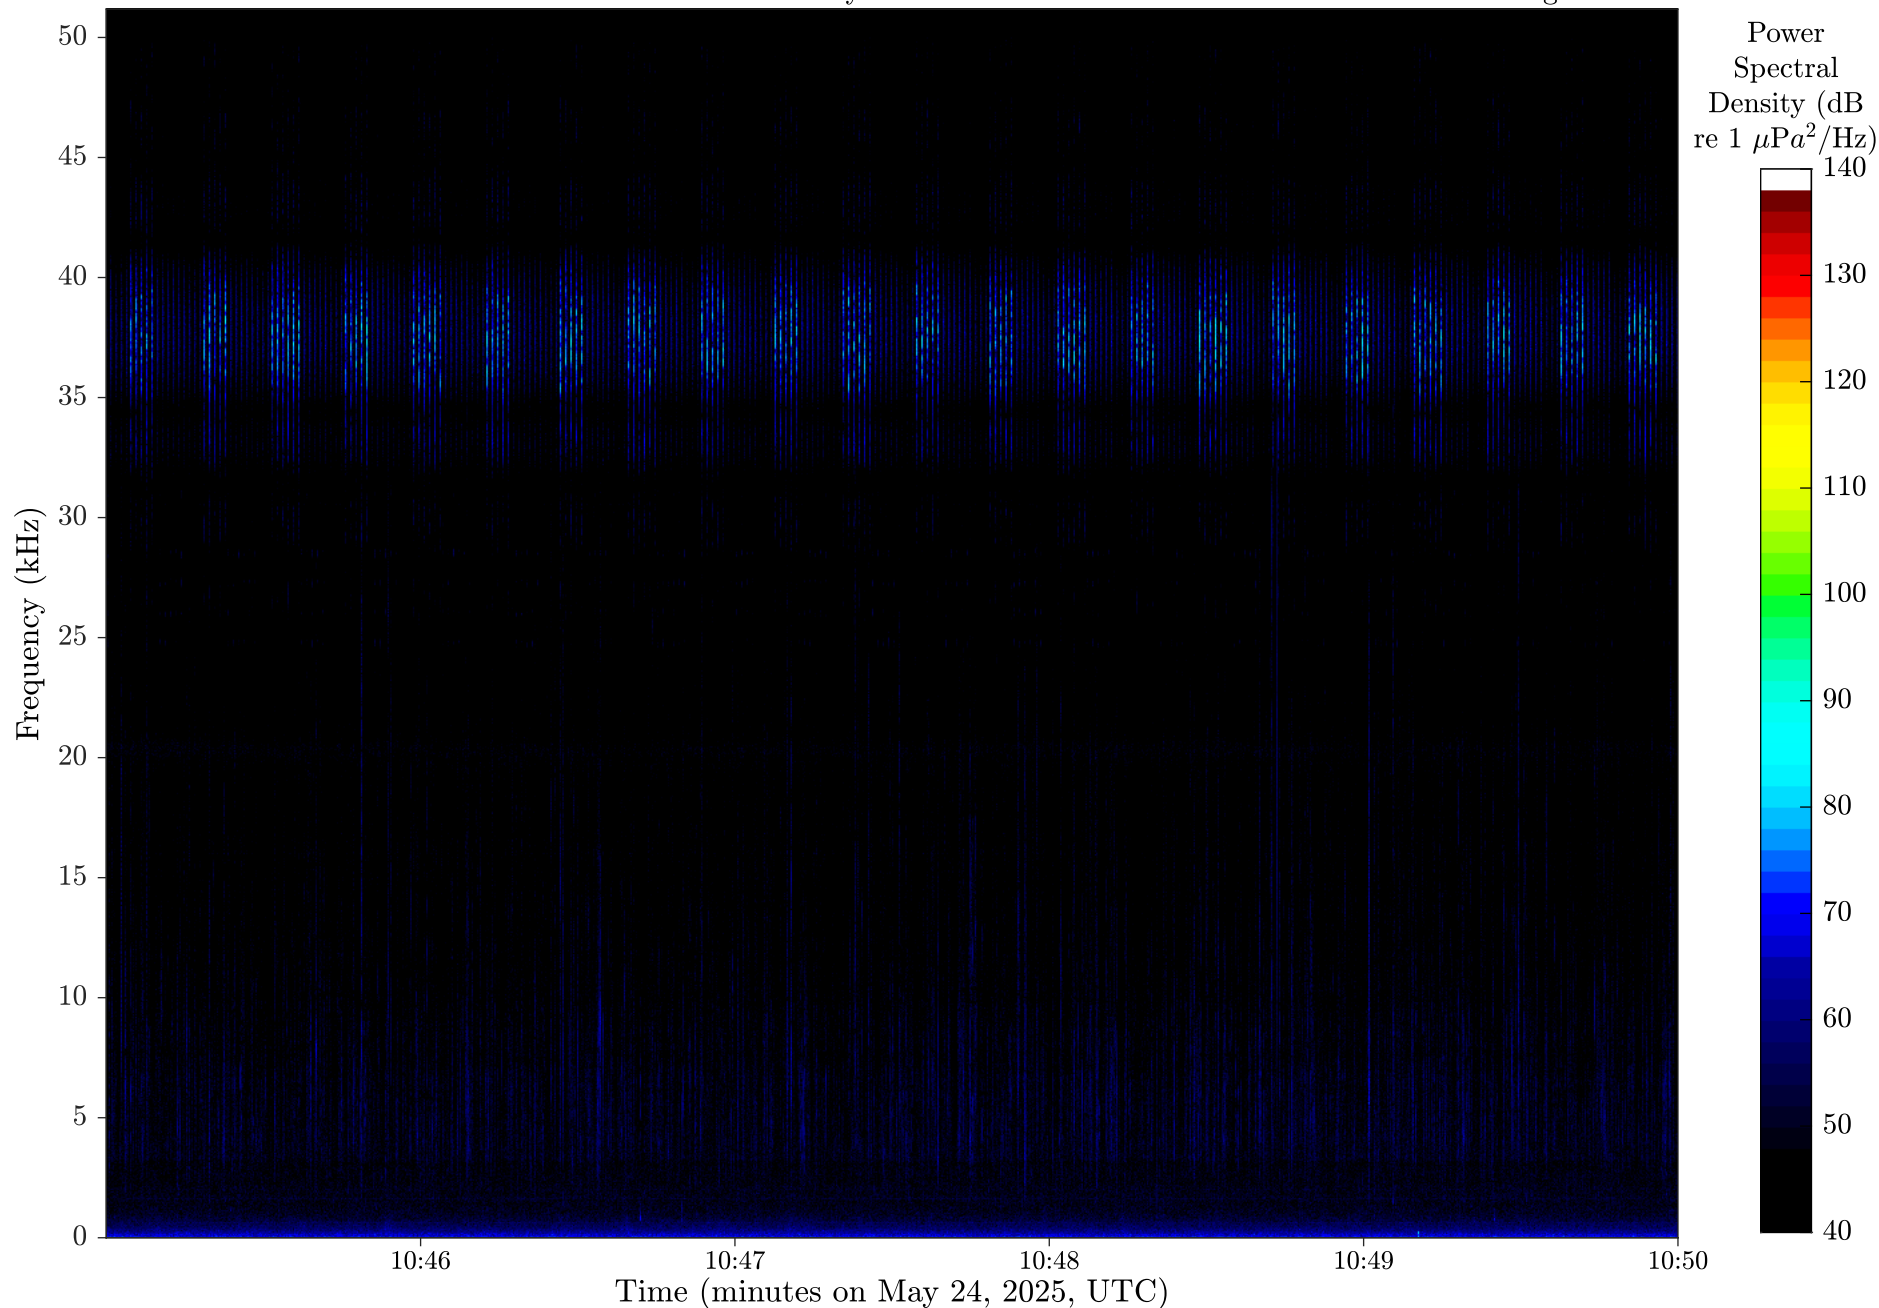


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:50 UTC

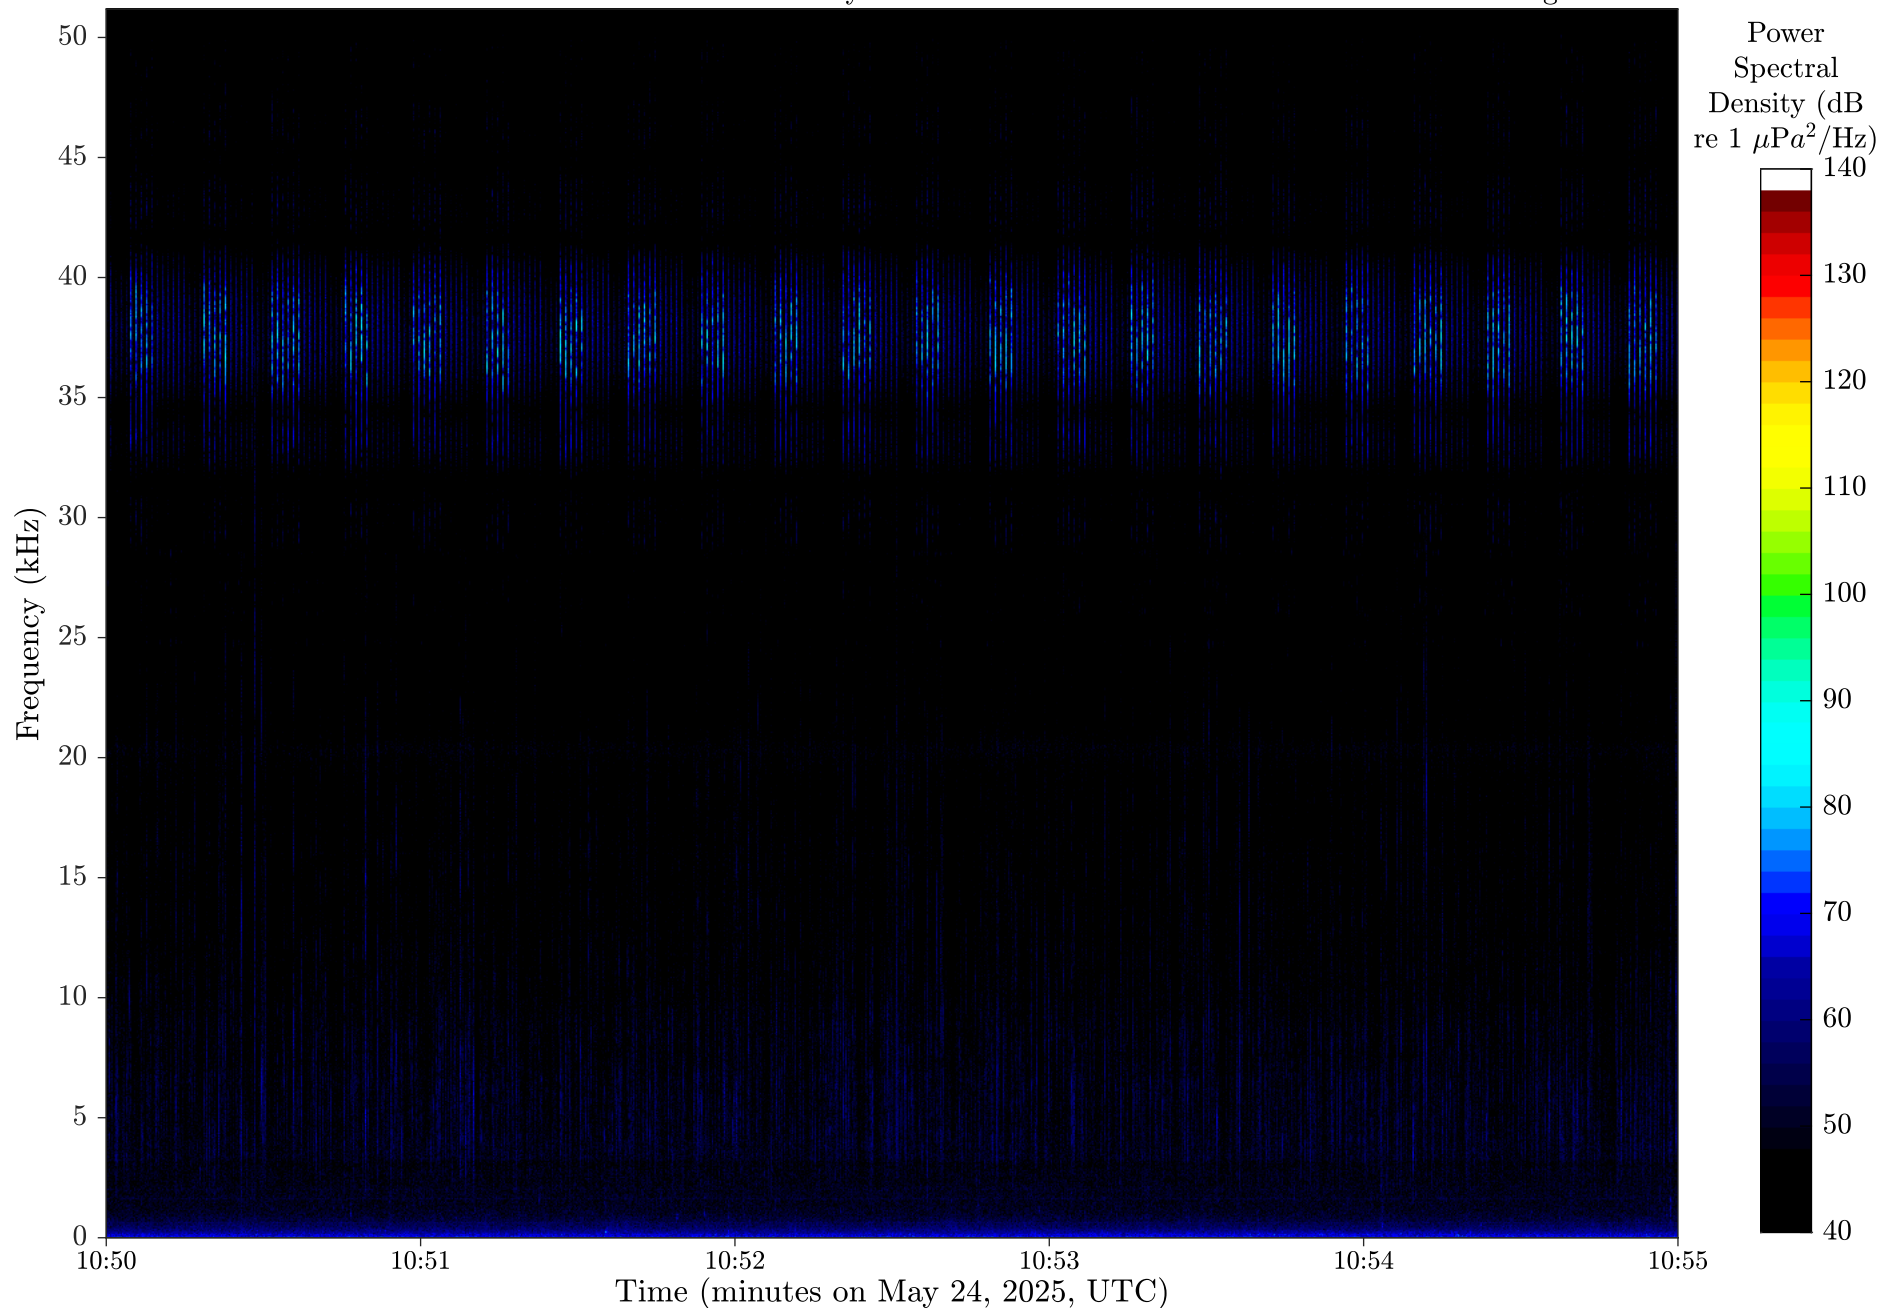


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:36:58 UTC

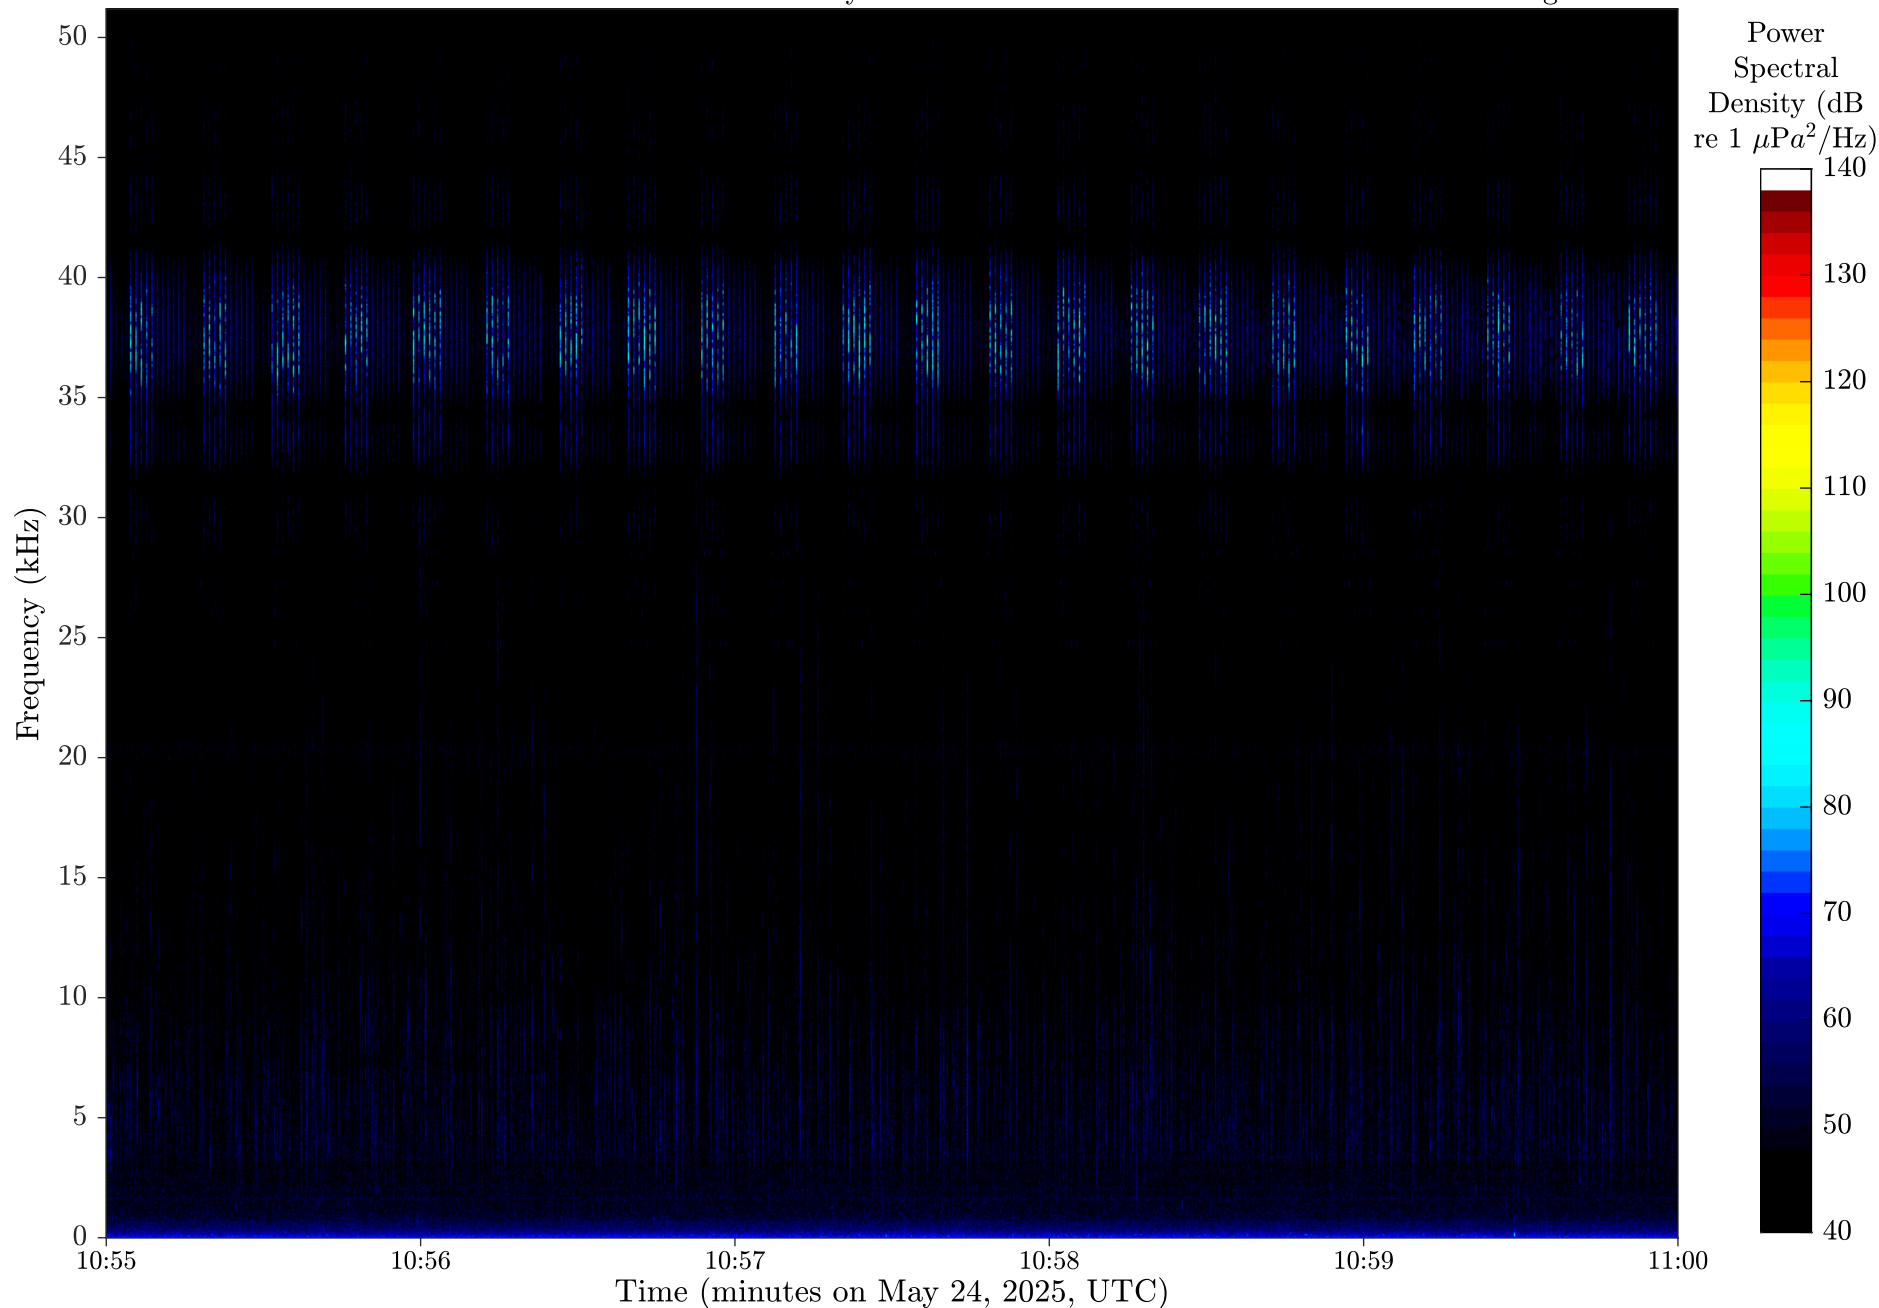

Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:05 UTC

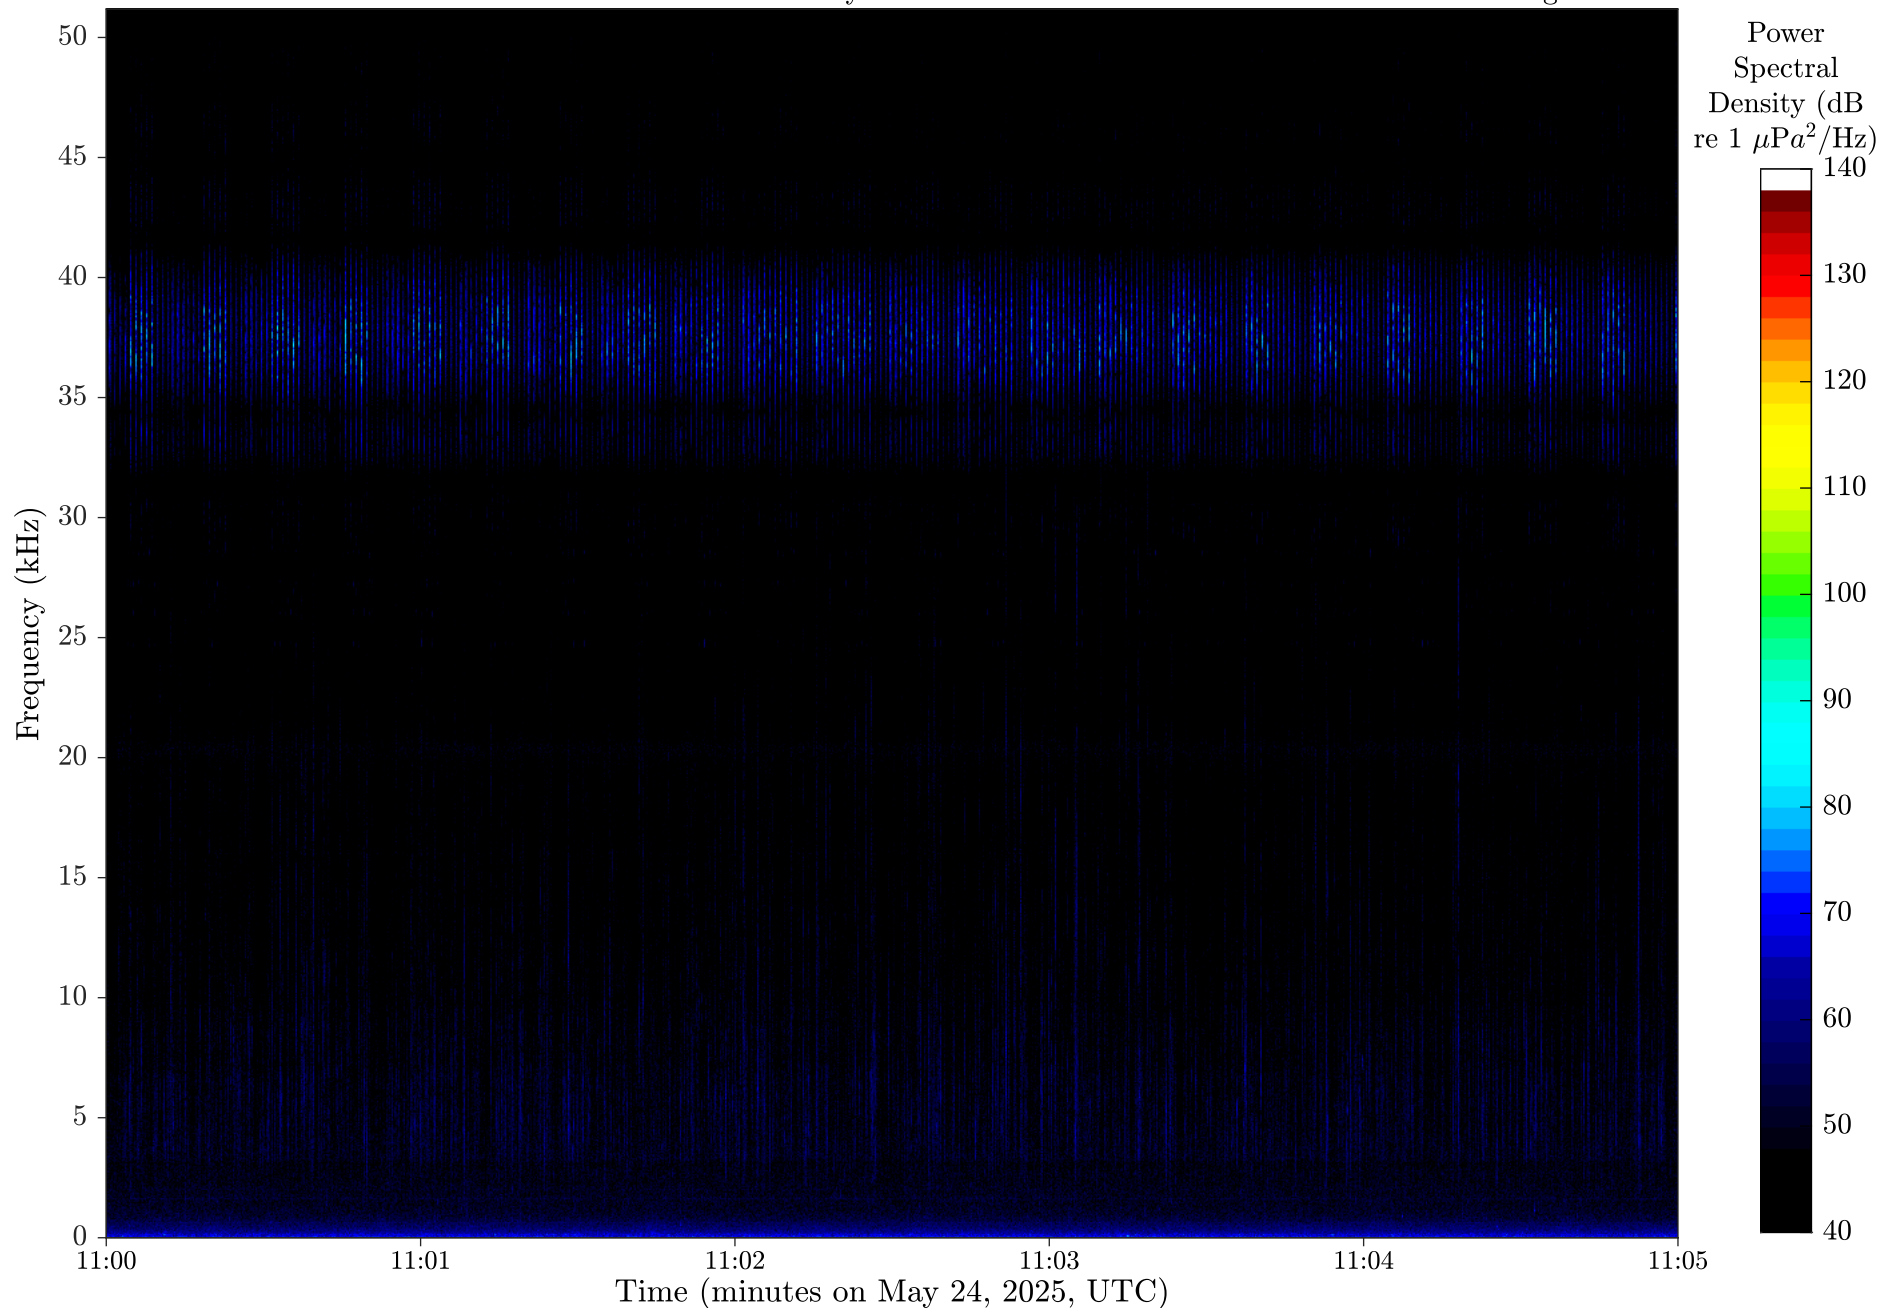


Comments: 32.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:37:13 UTC

Ocean Sonics icListen HF Hydrophone 1266 (23235)
Folger Passage • Folger Deep • 48.8139° N • 125.2746° W • 95 m
Start time: 24-May-2025 11:05:00.000 UTC • Data Diversion Mode: Original Data




Comments: 23.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

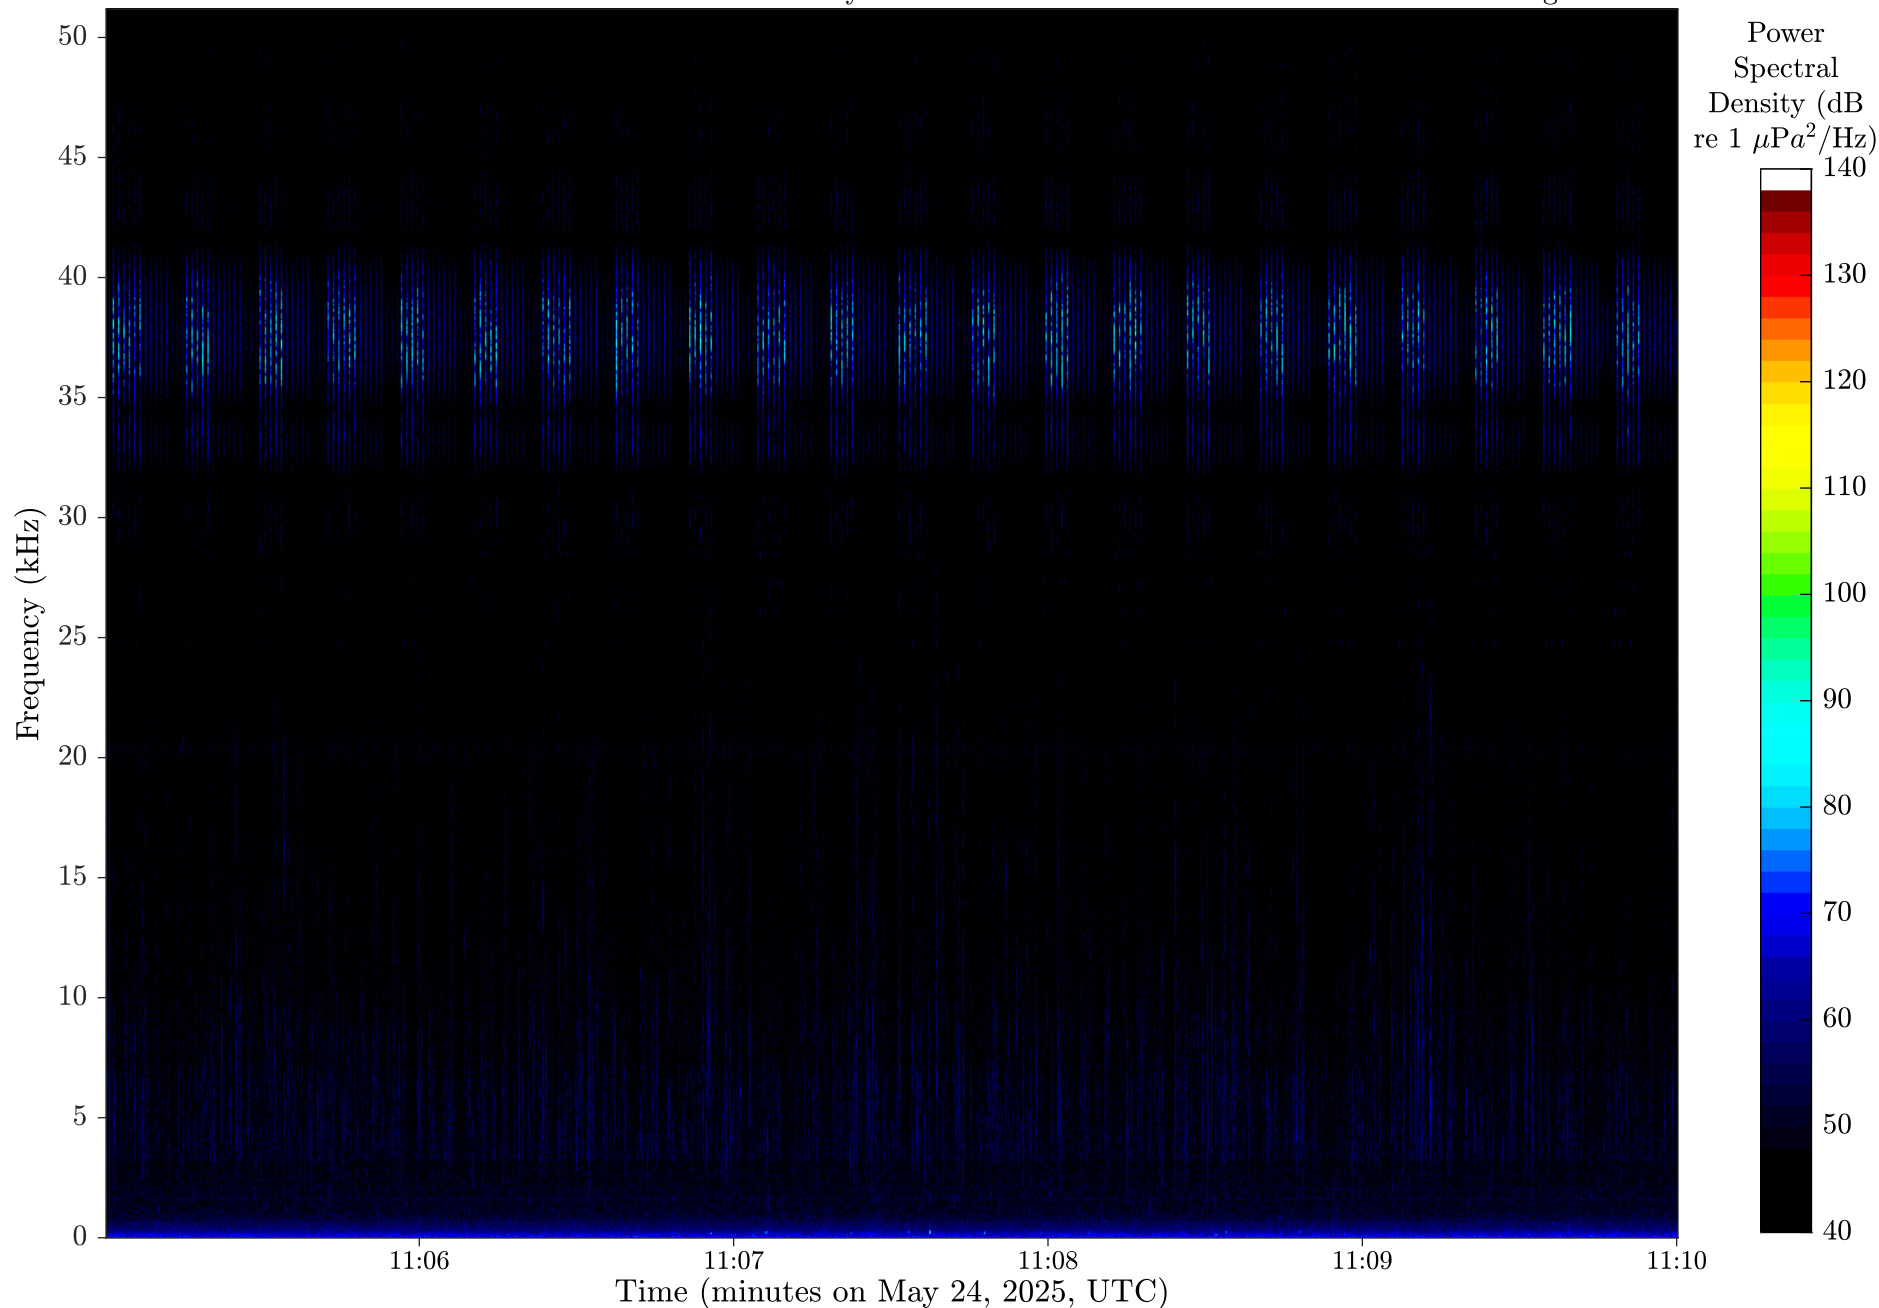

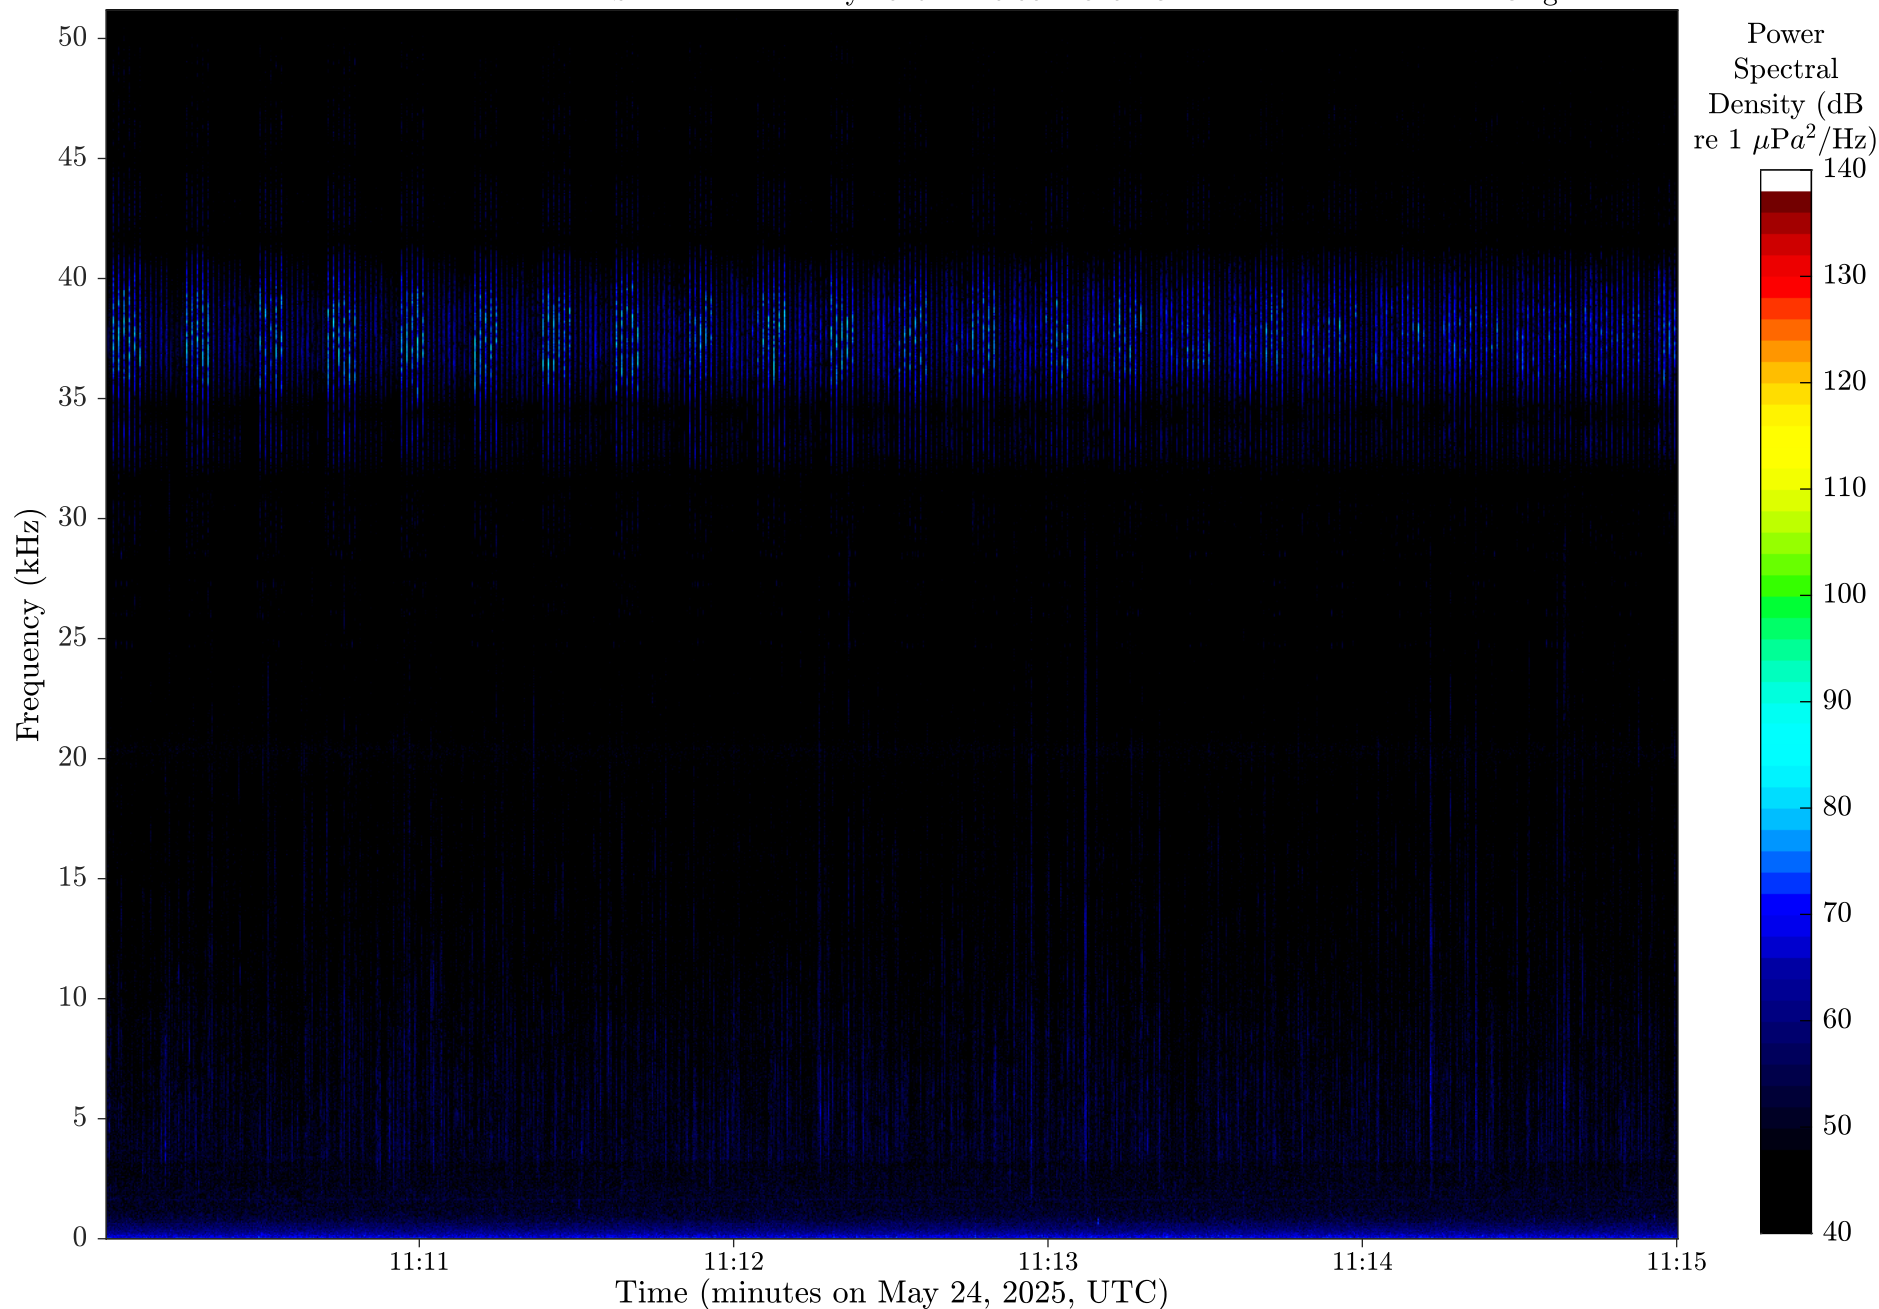


Comments: 32.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:37:29 UTC

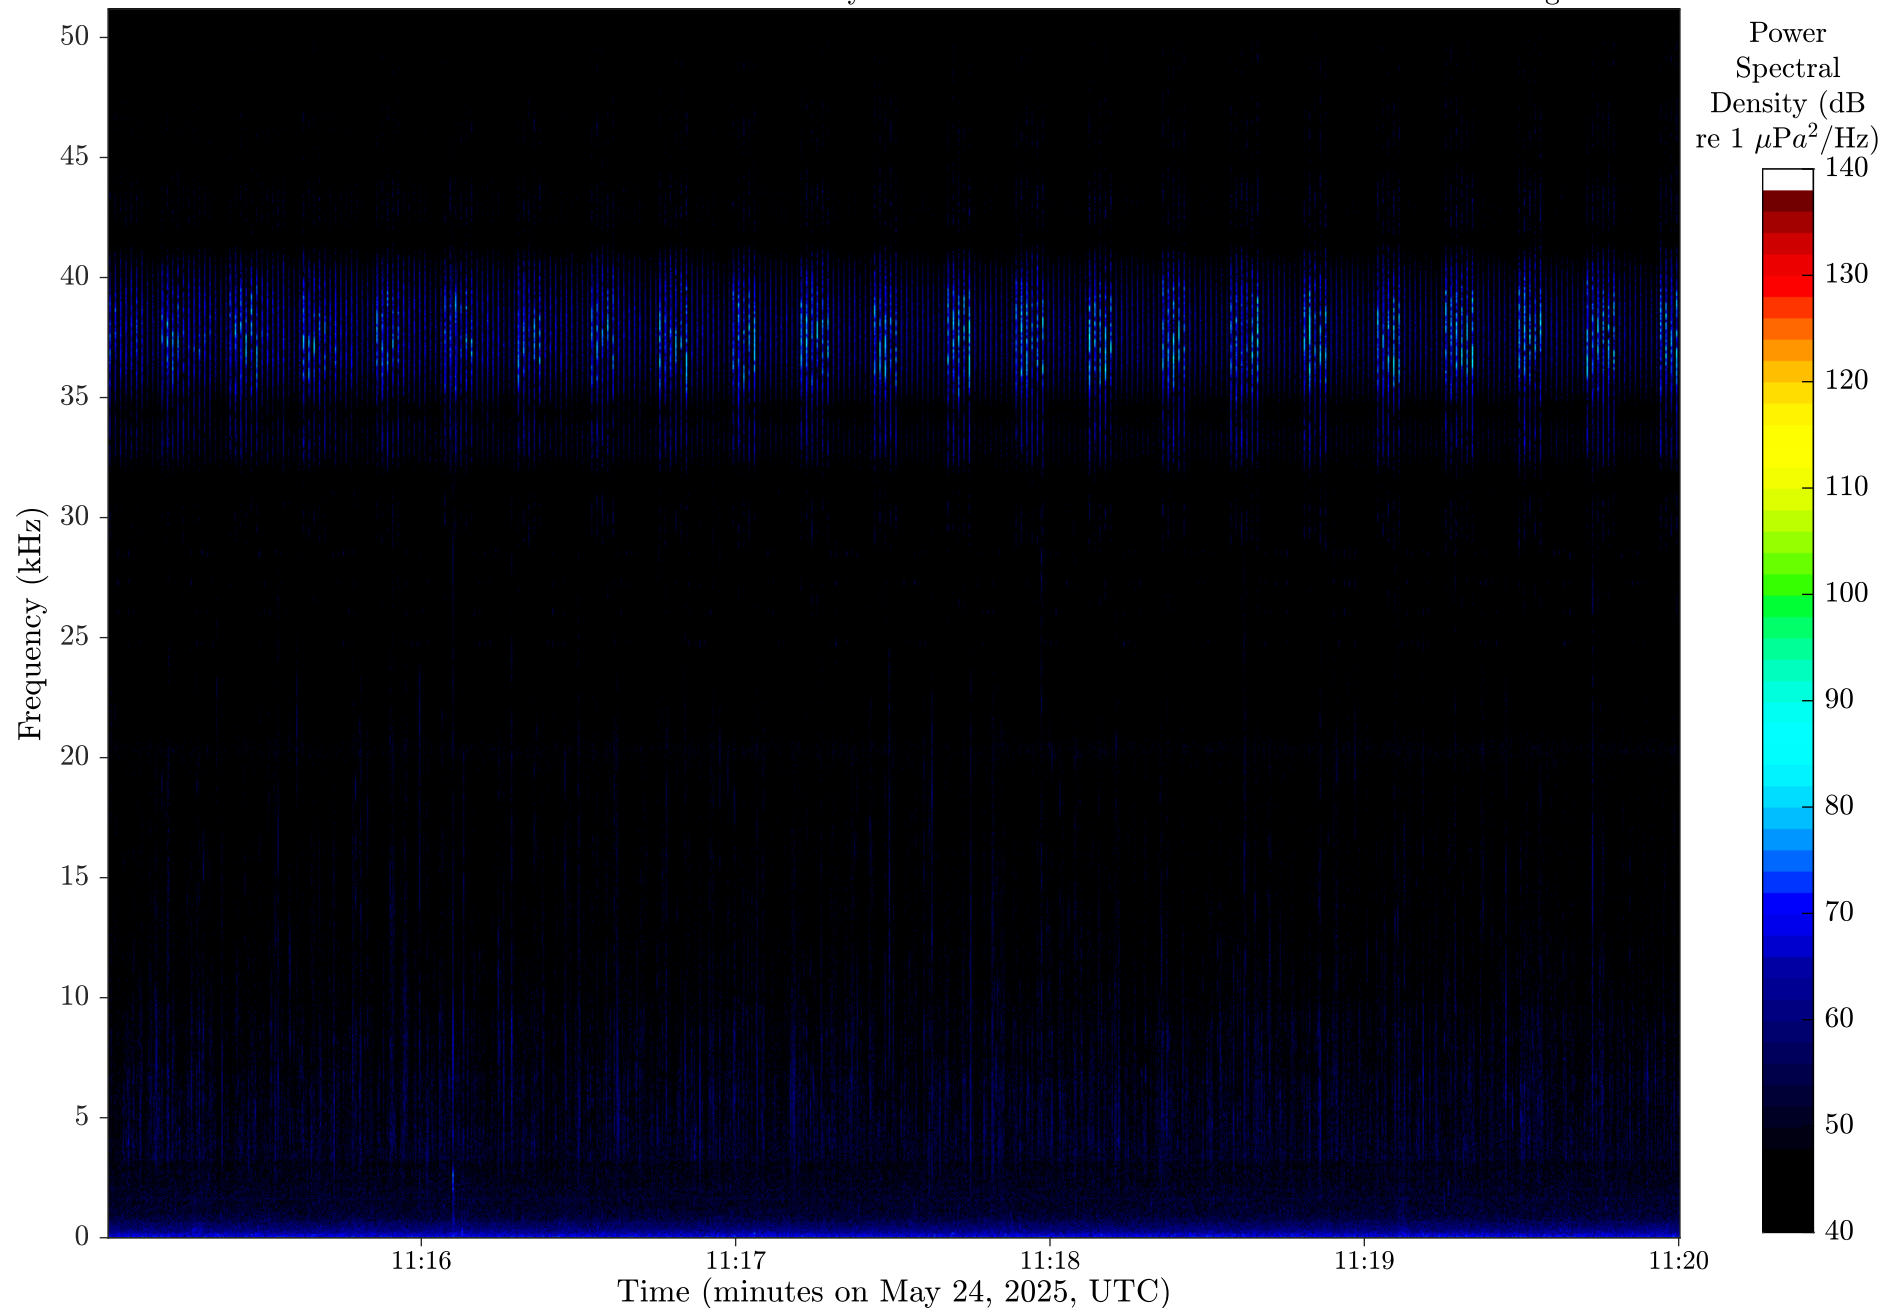


Comments: 31.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:37:37 UTC

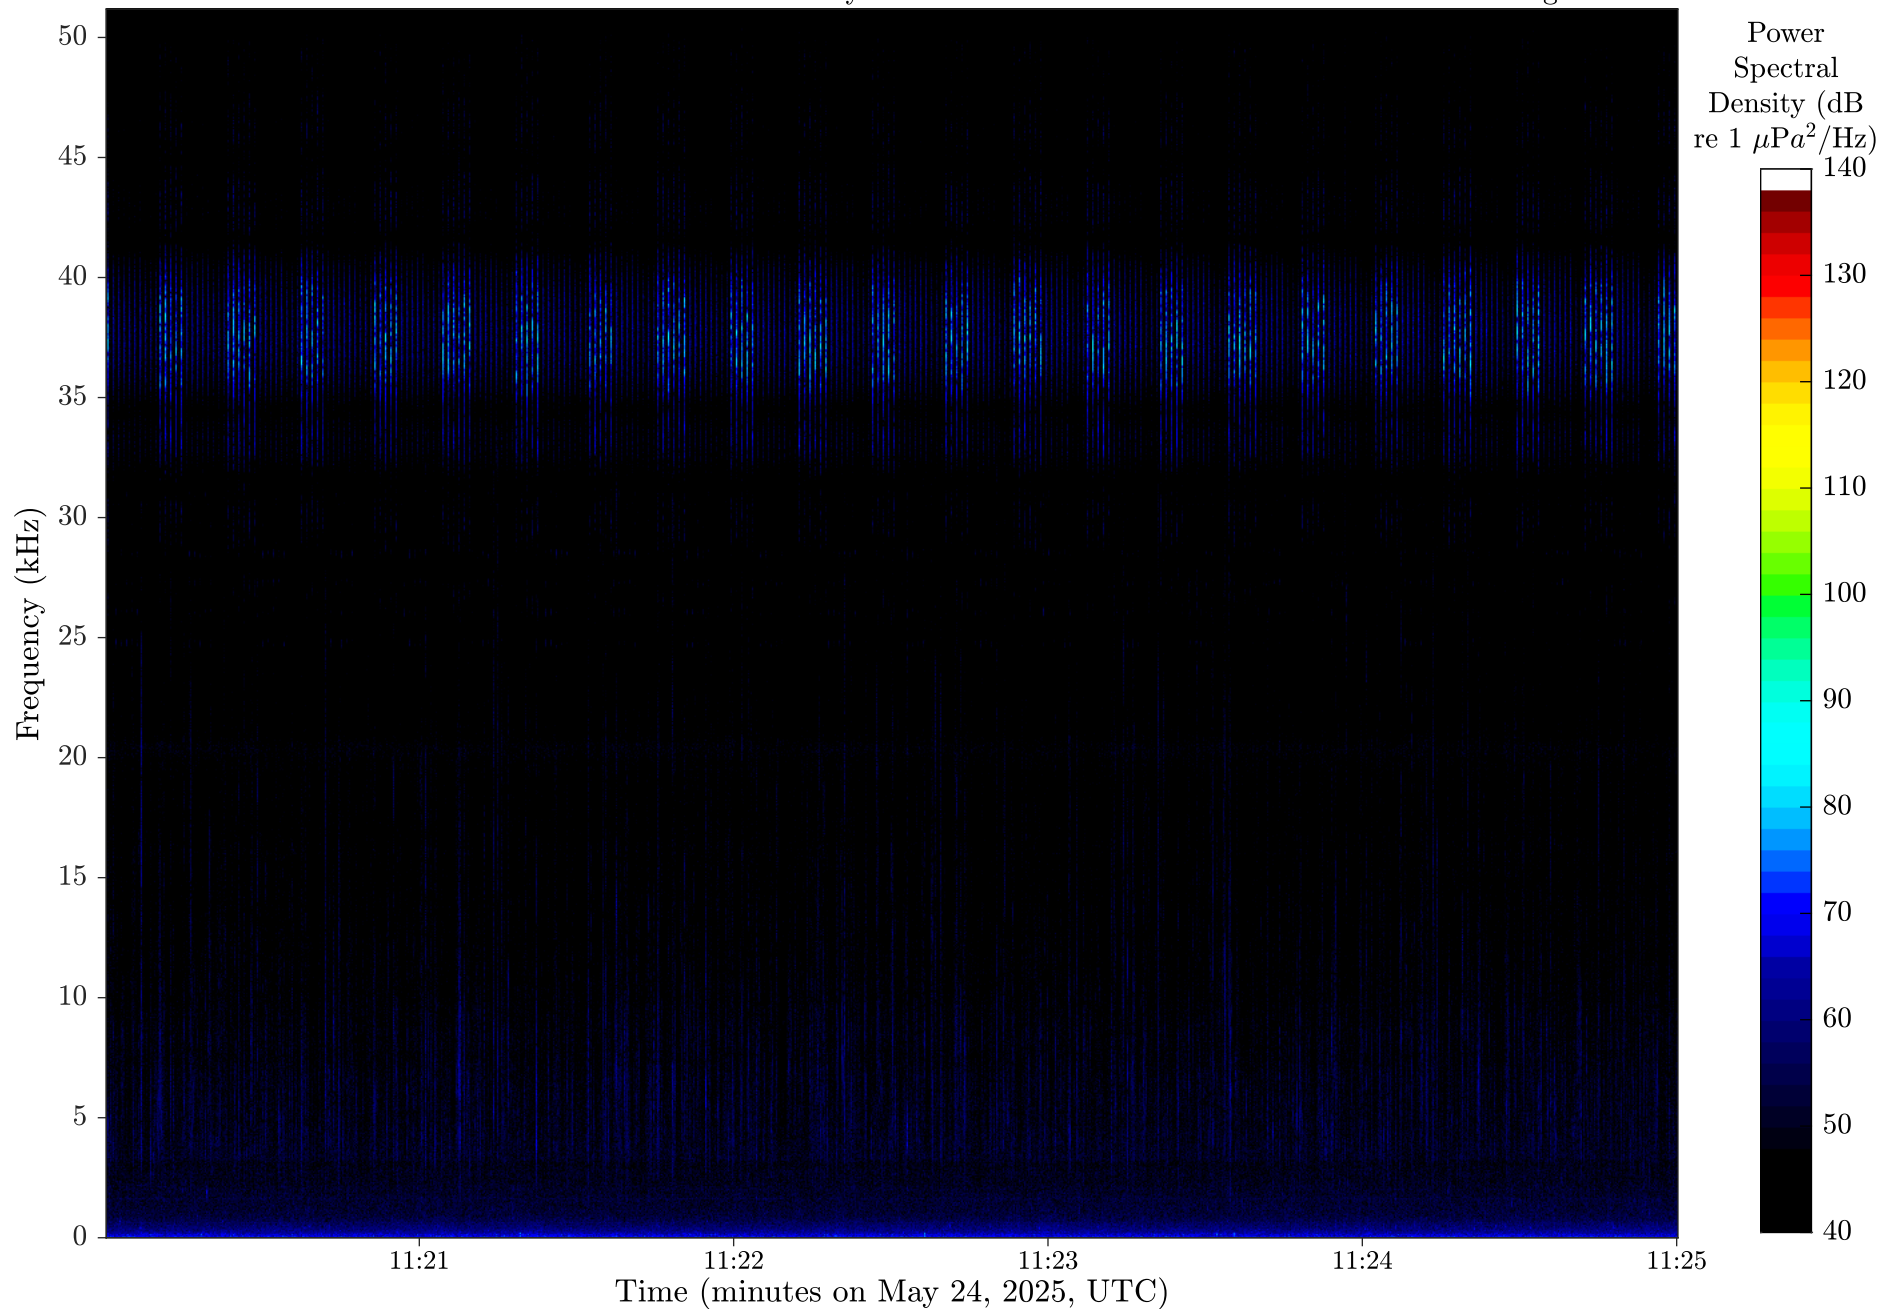


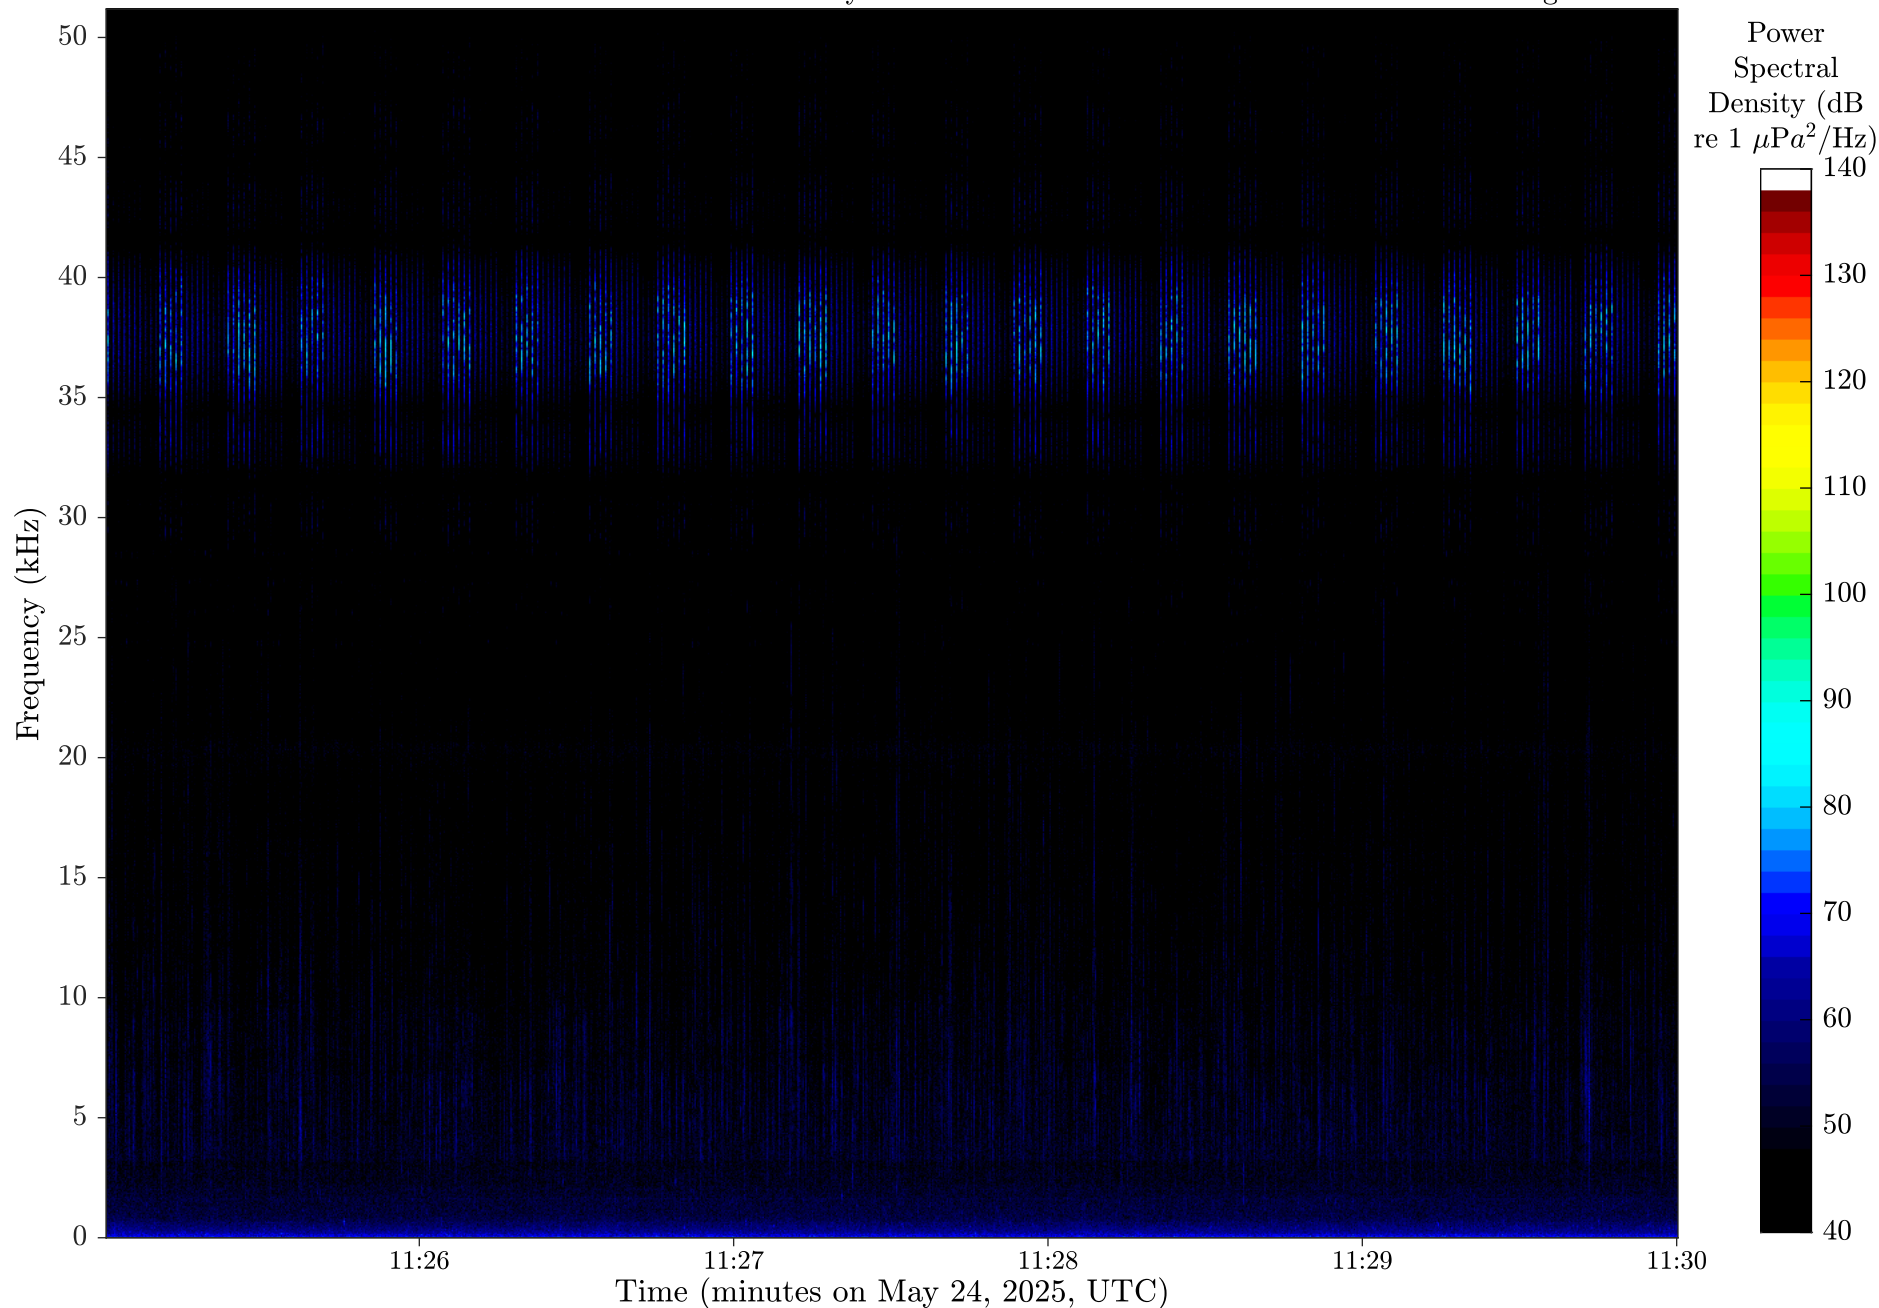


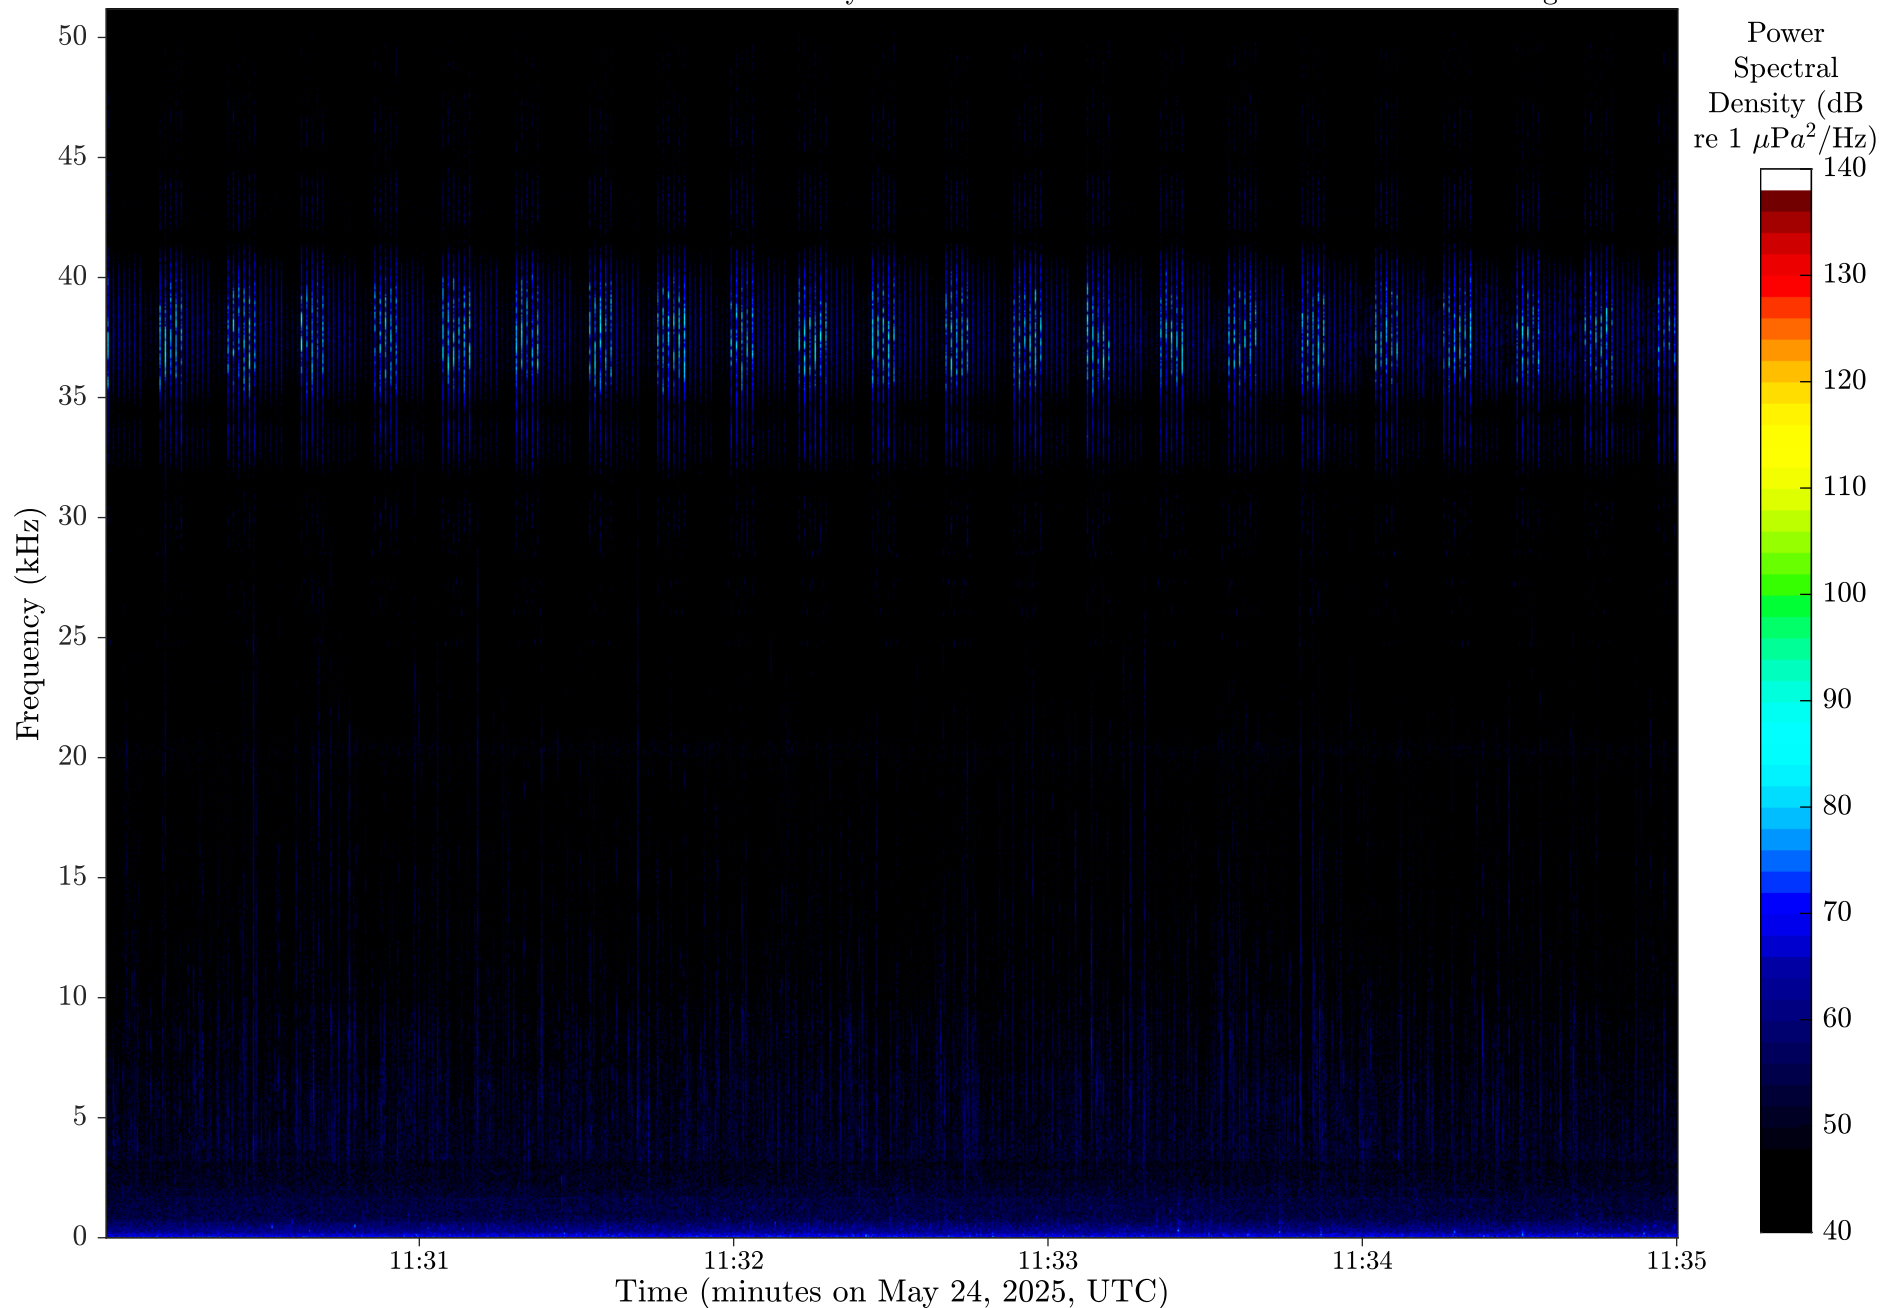

Comments: 32.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:38:00 UTC

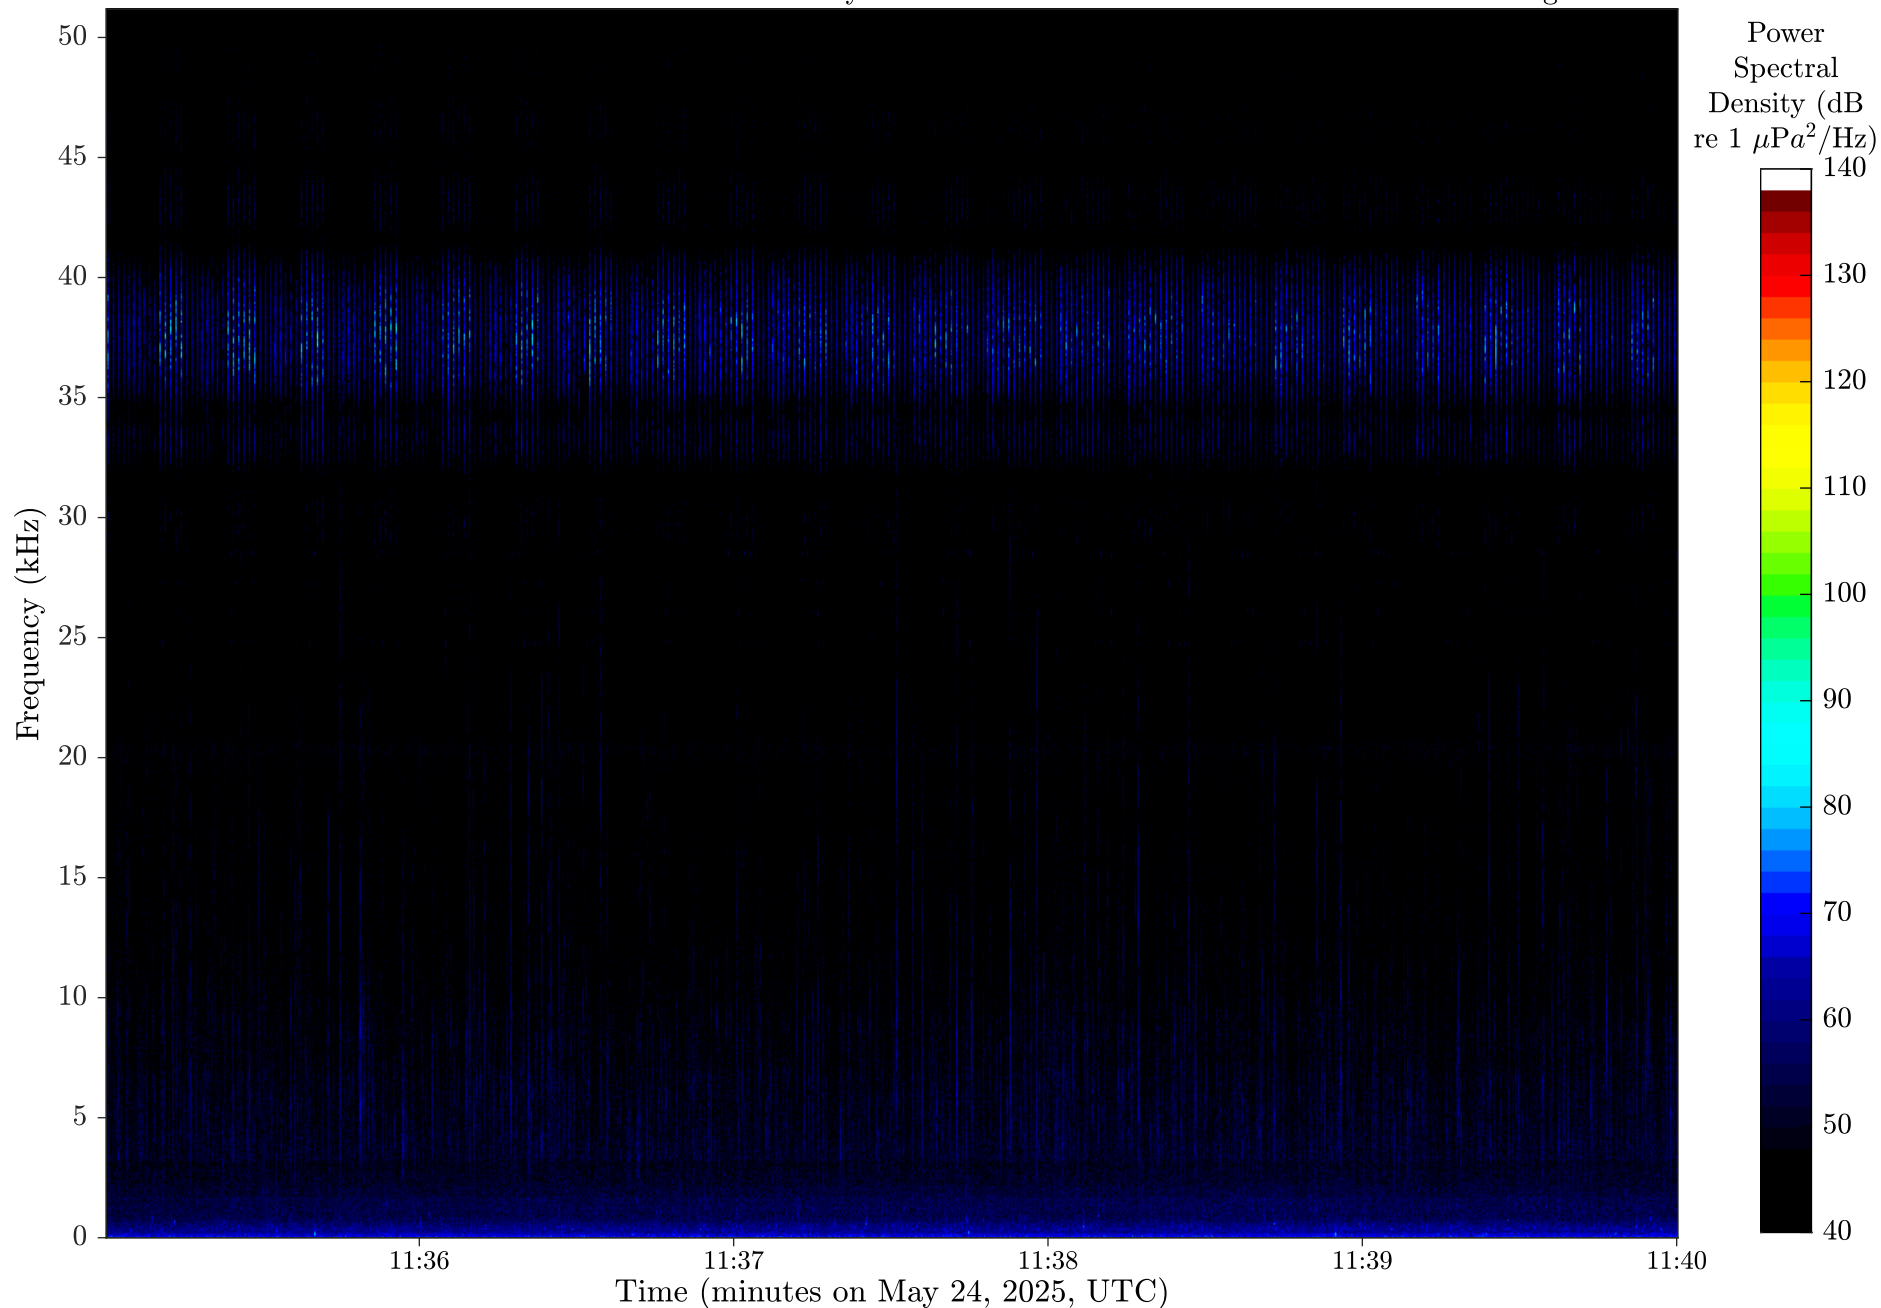


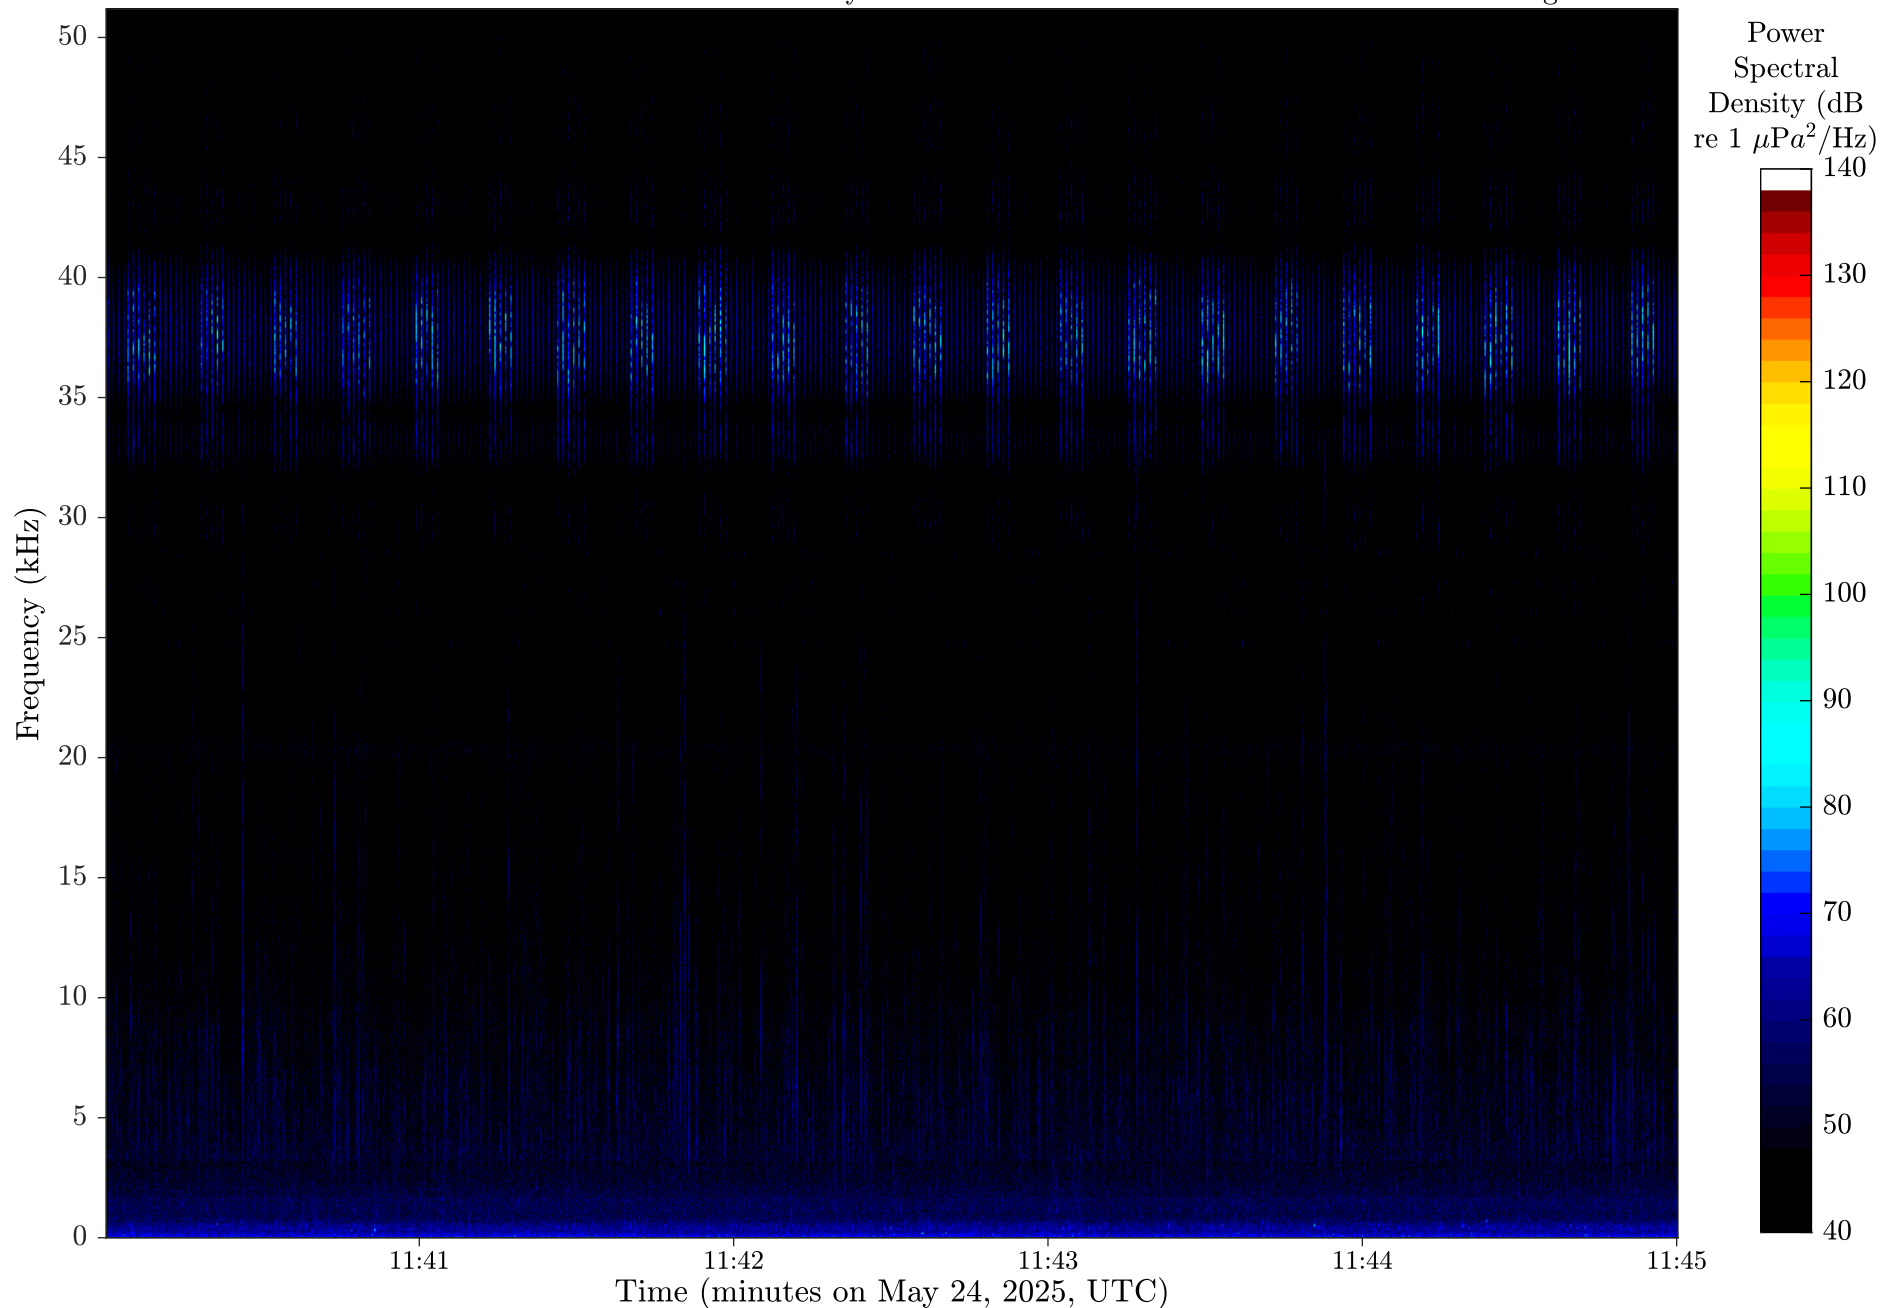

Comments: 30.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:38:15 UTC

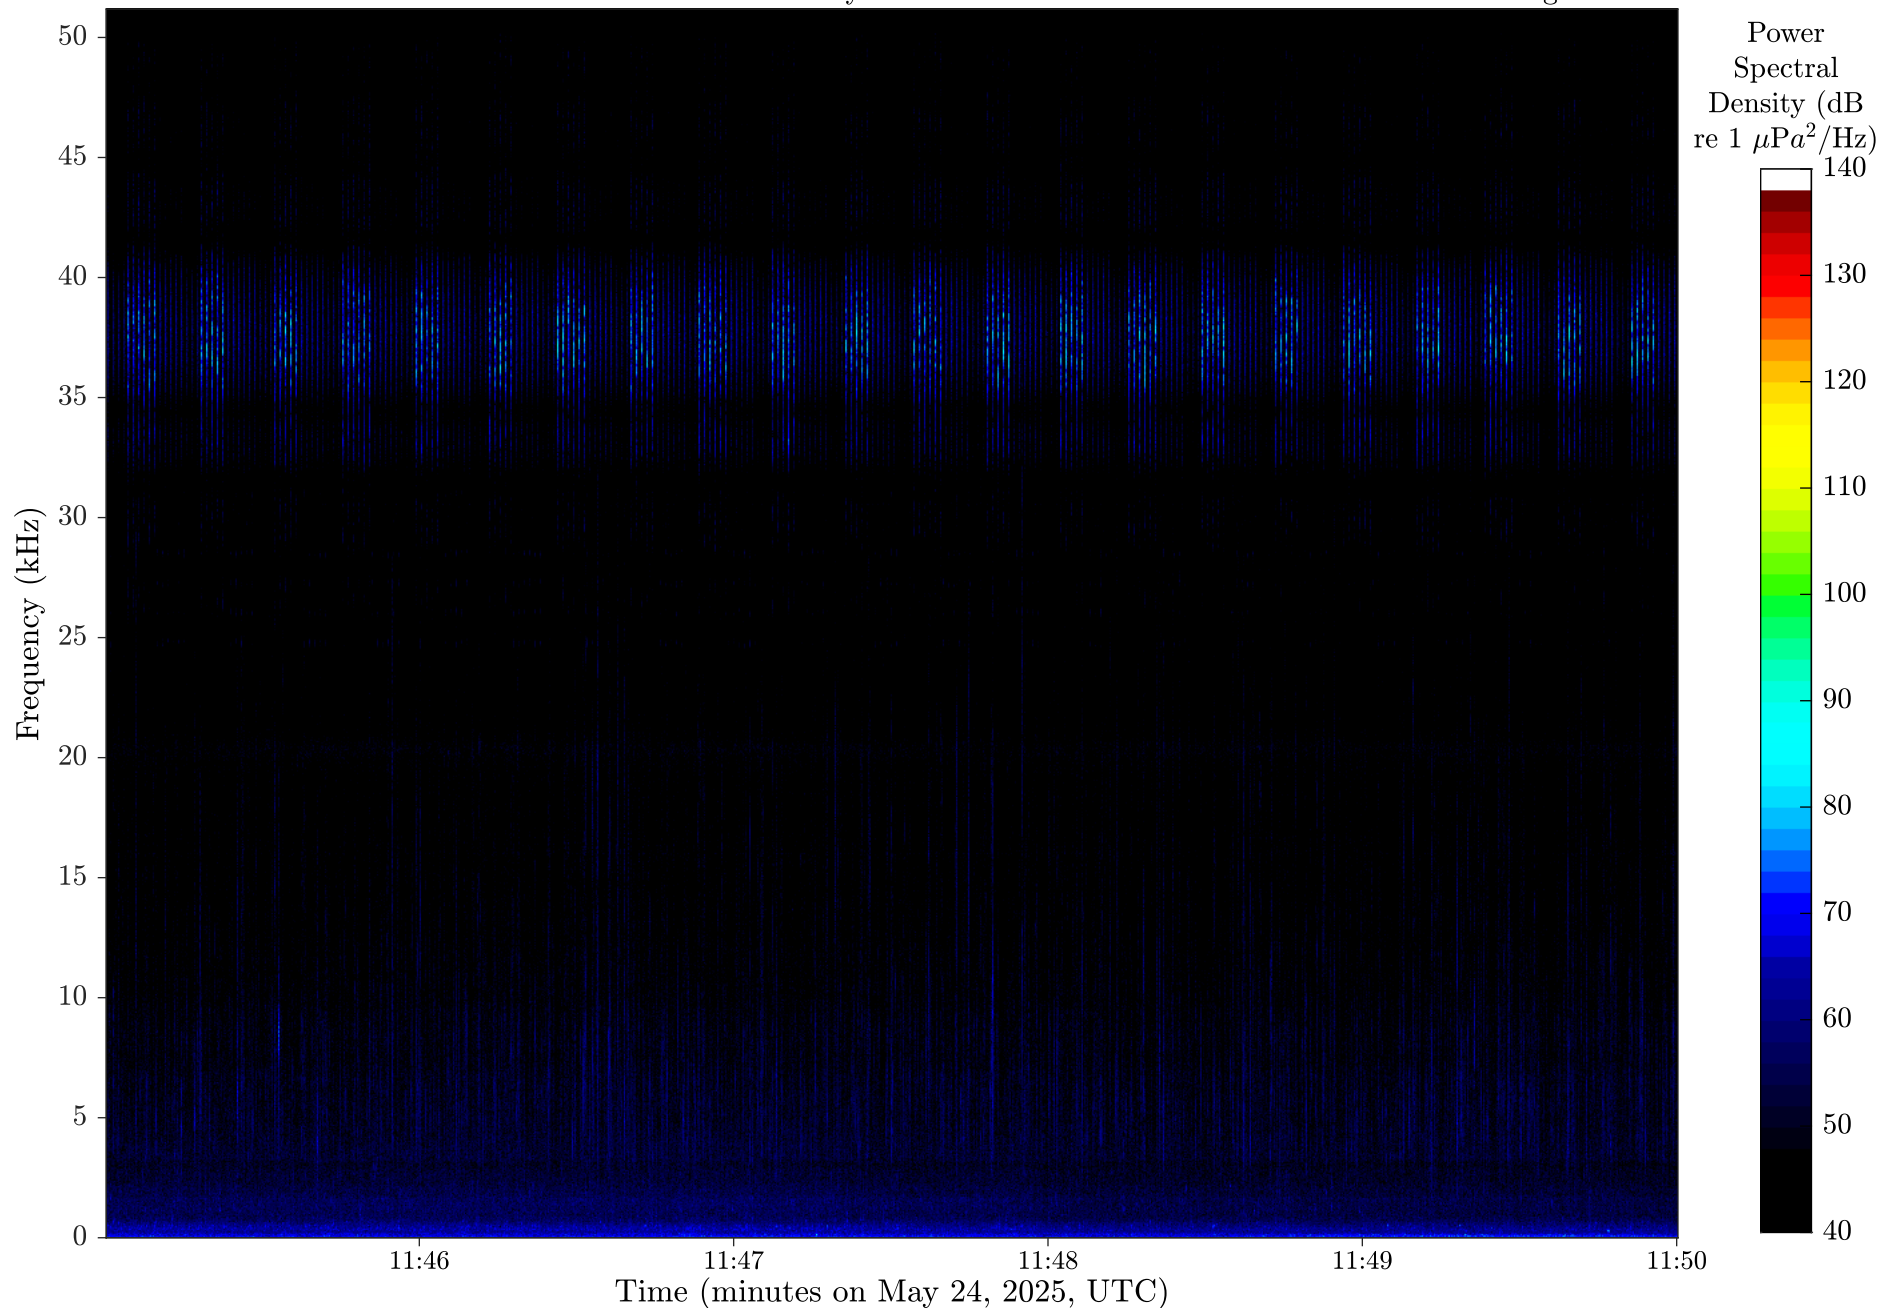

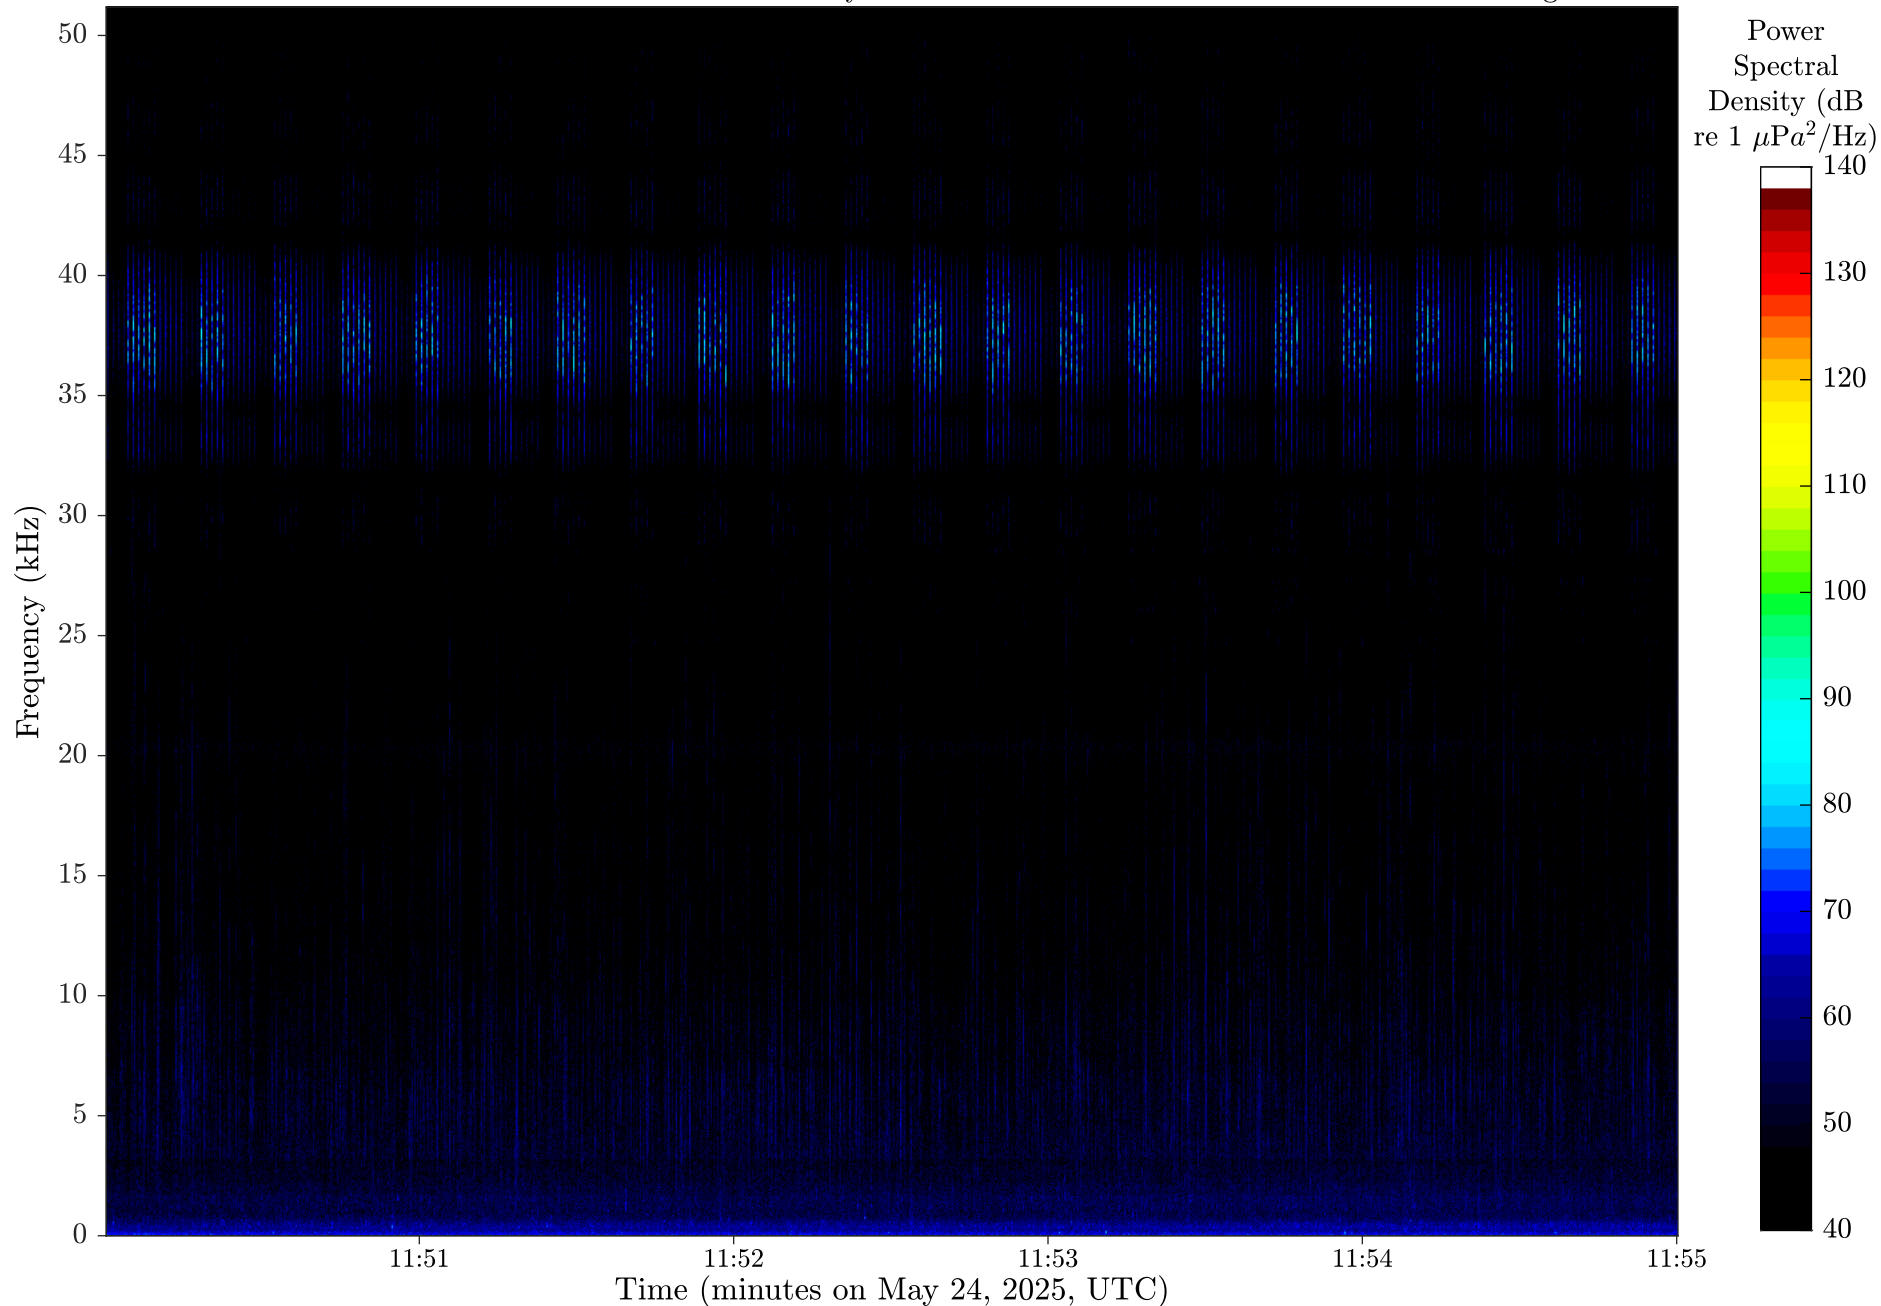


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:38:30 UTC

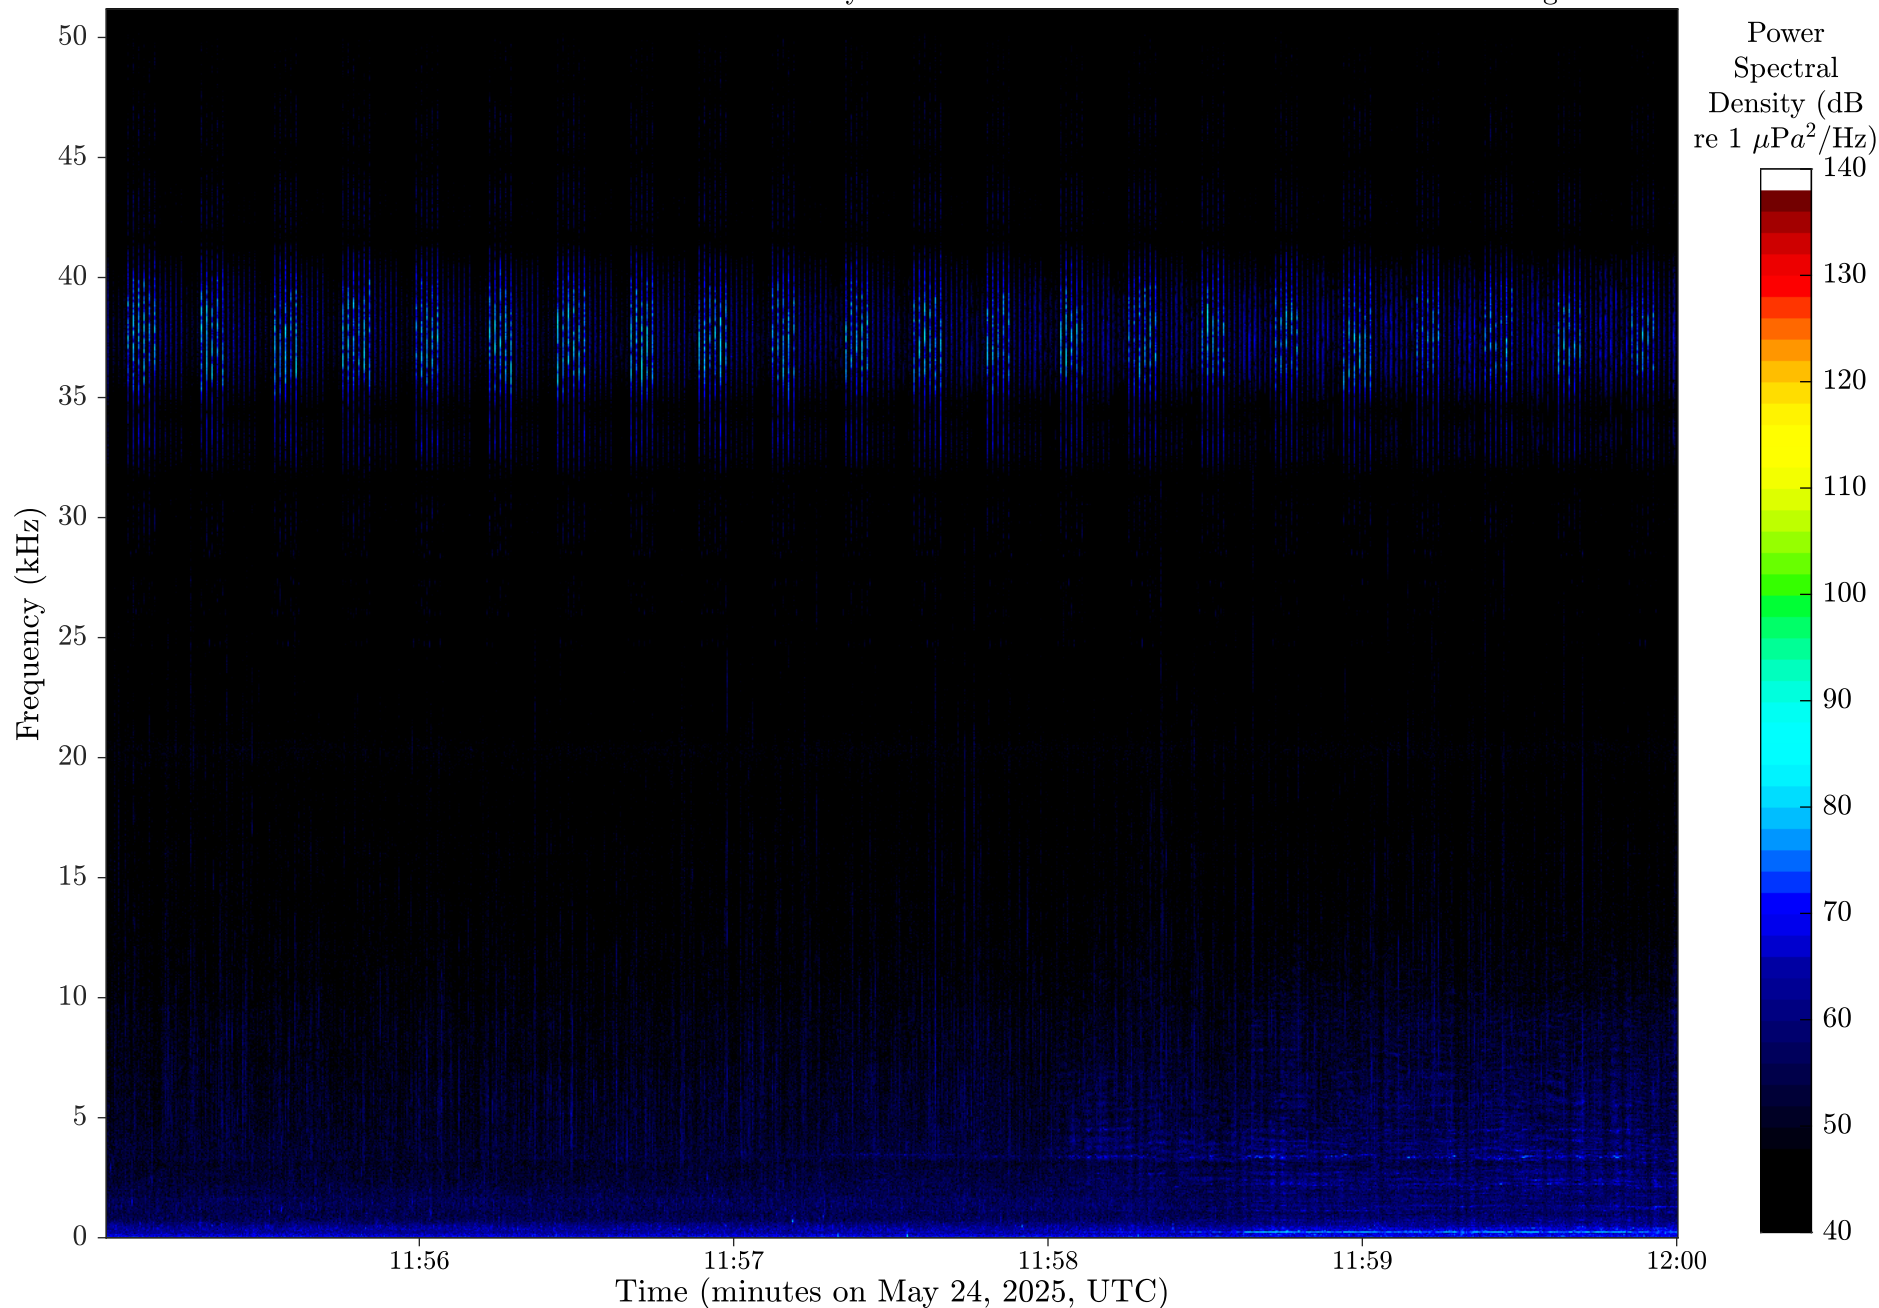

Comments: 31 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:38:38 UTC

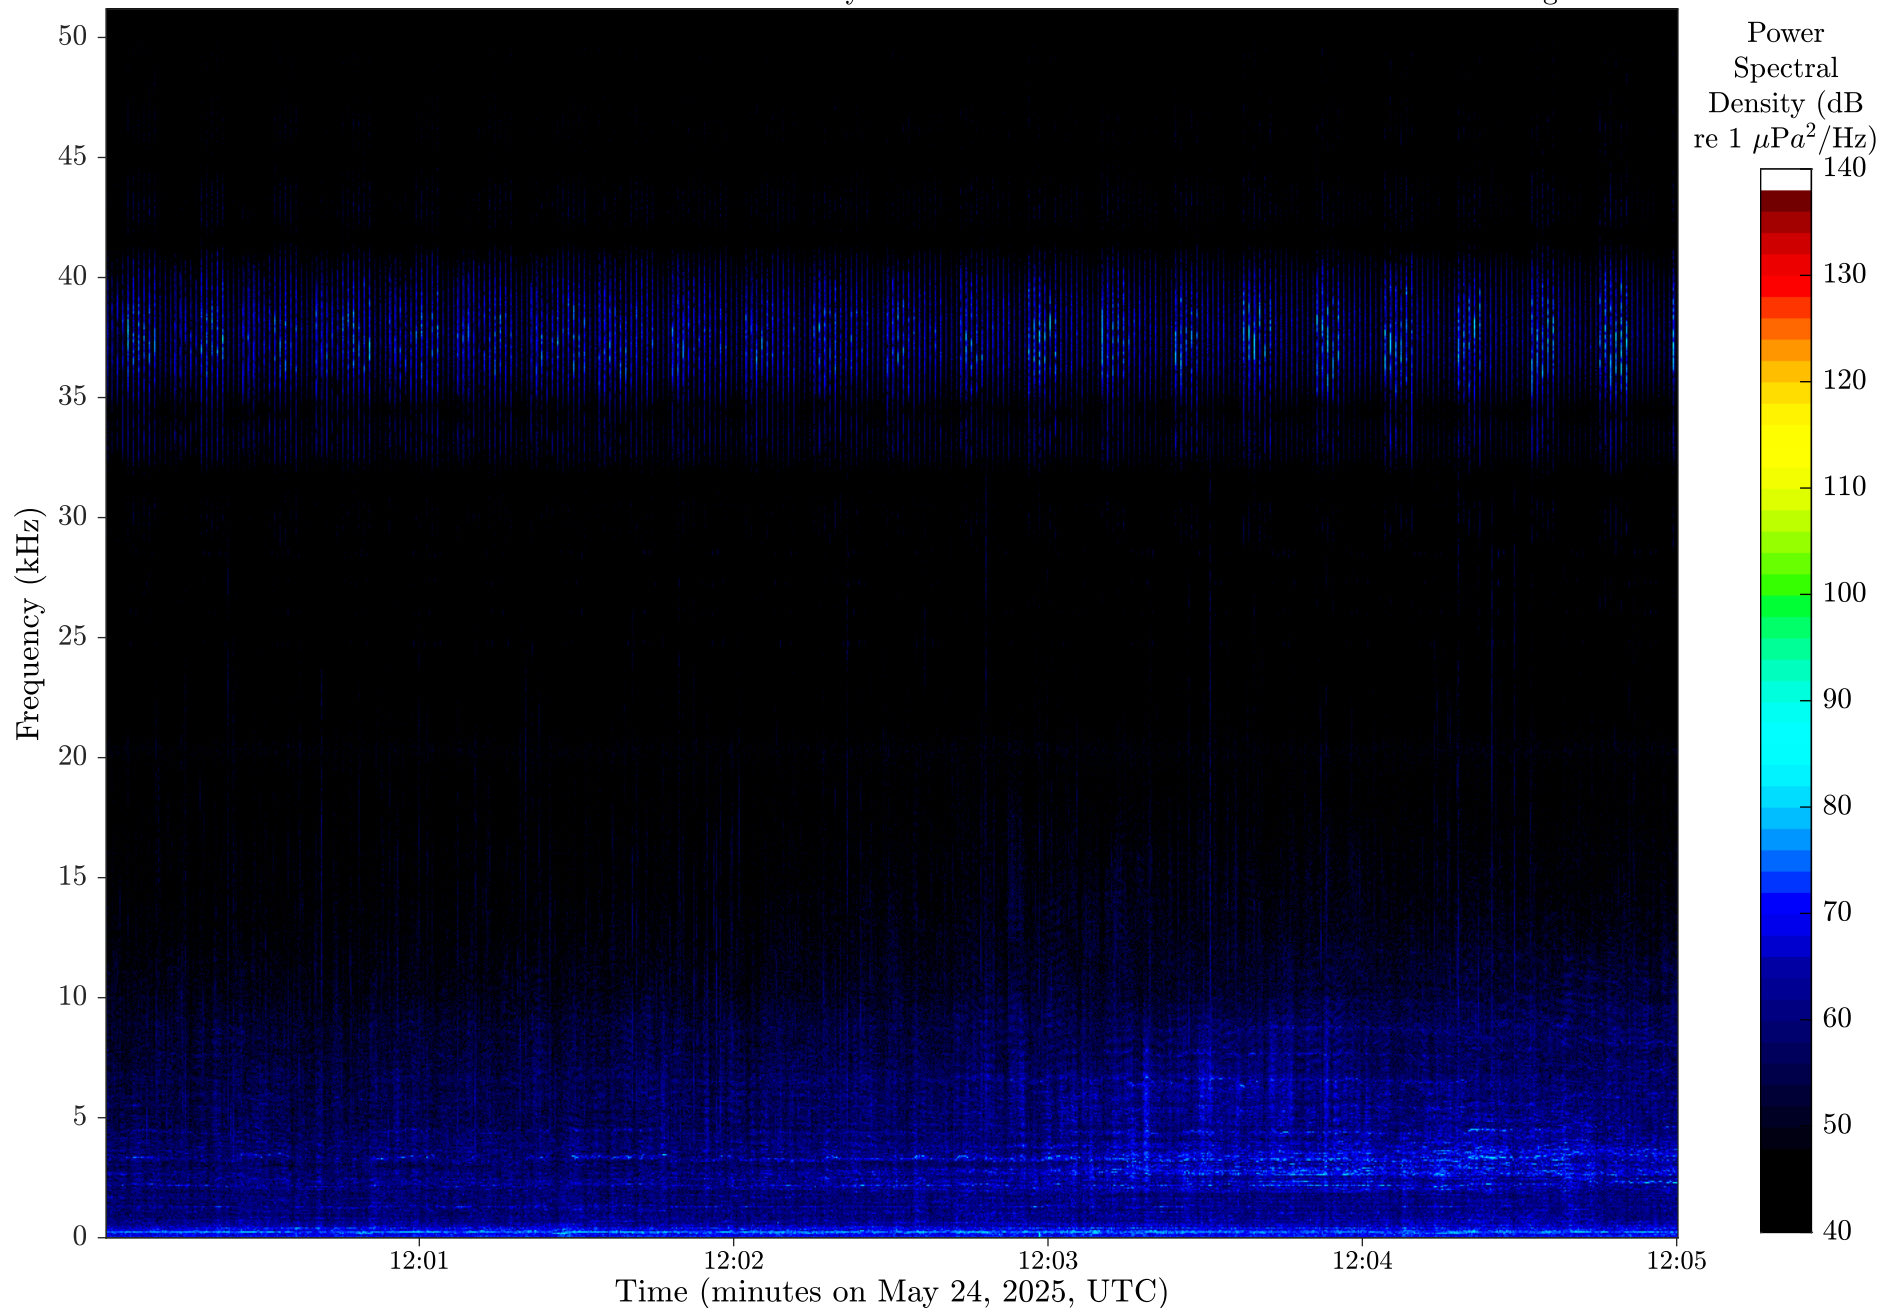

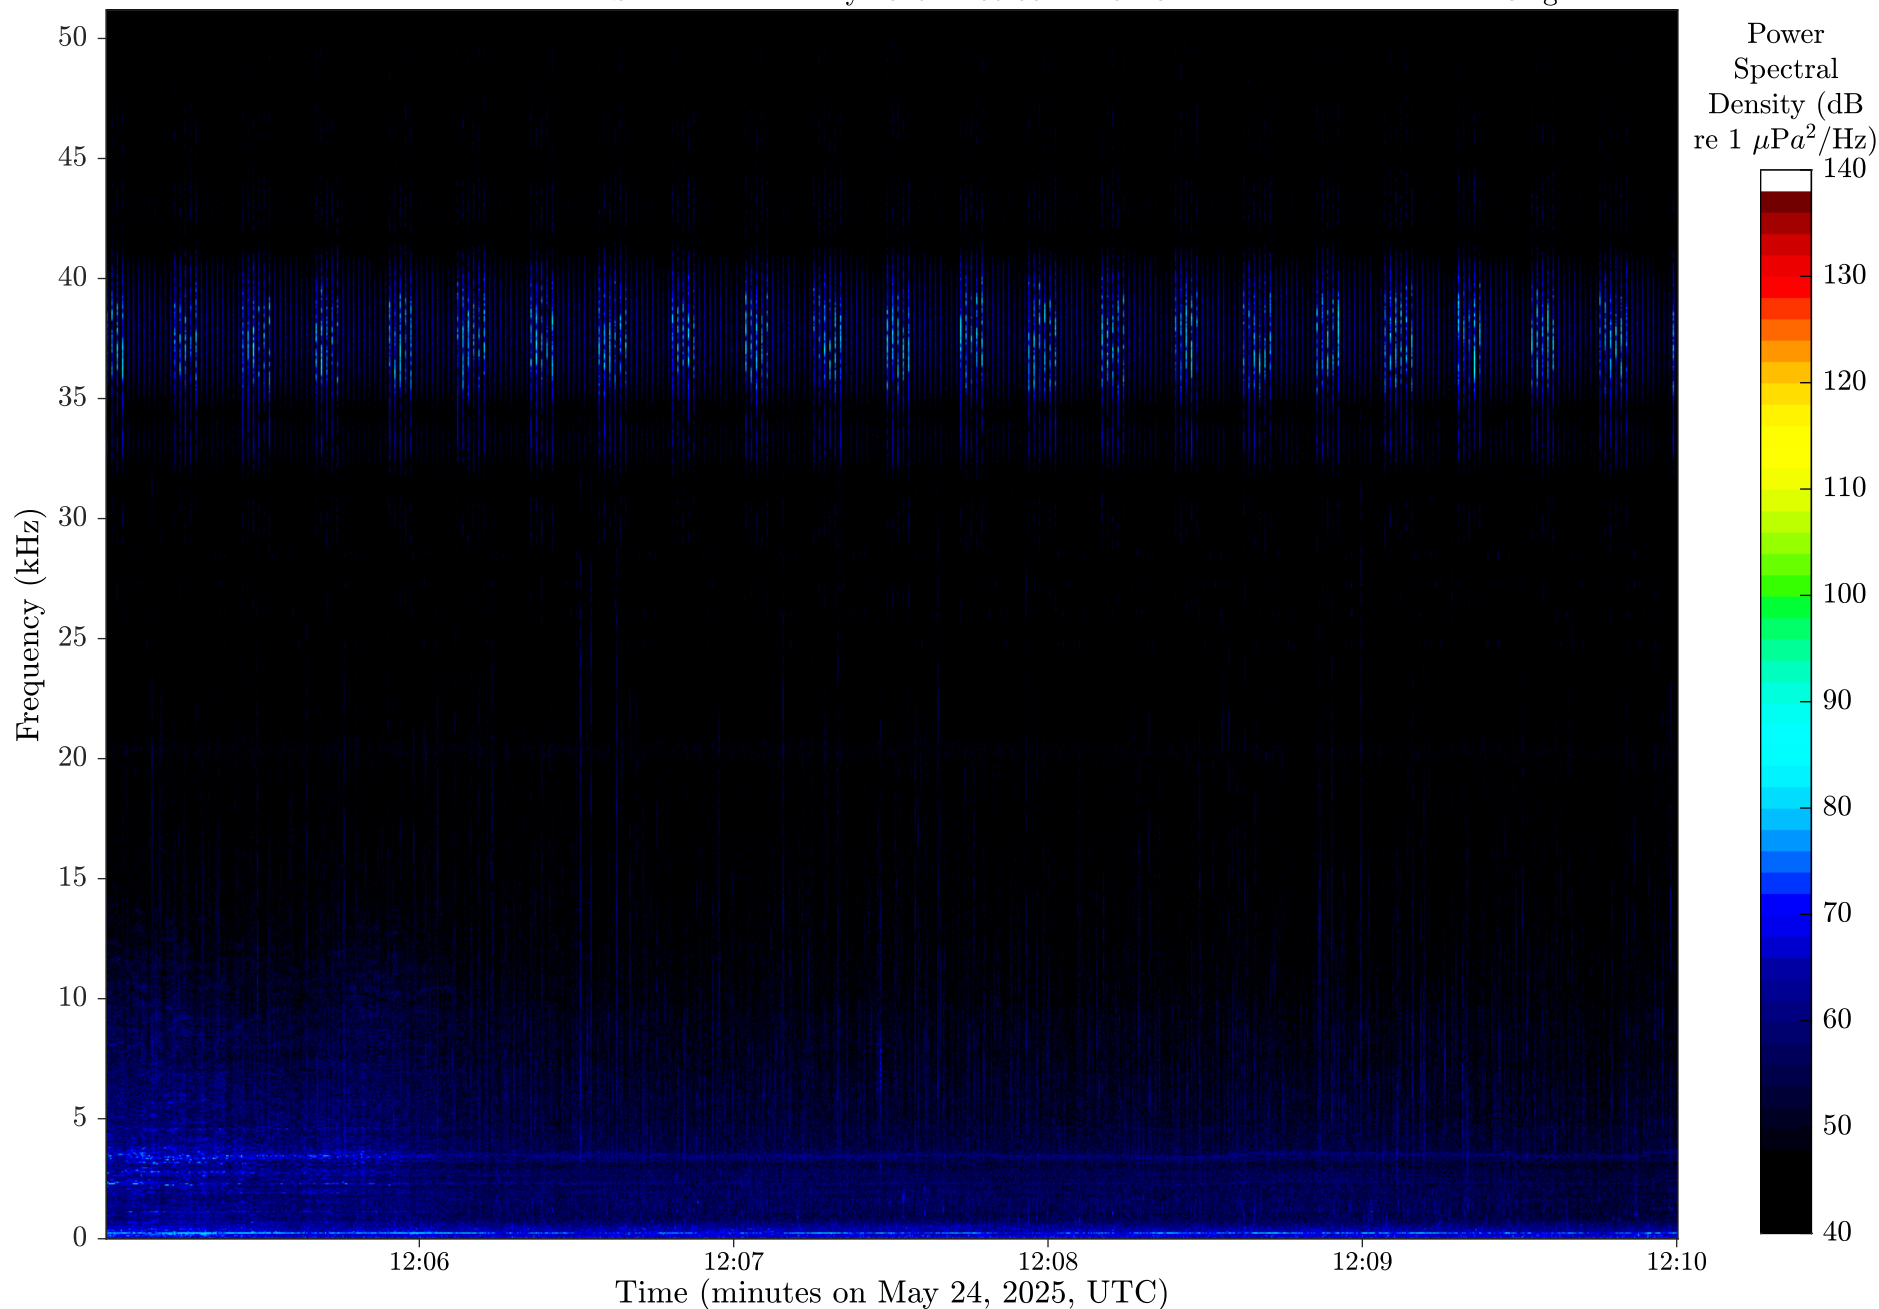


Comments: 29.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:38:54 UTC

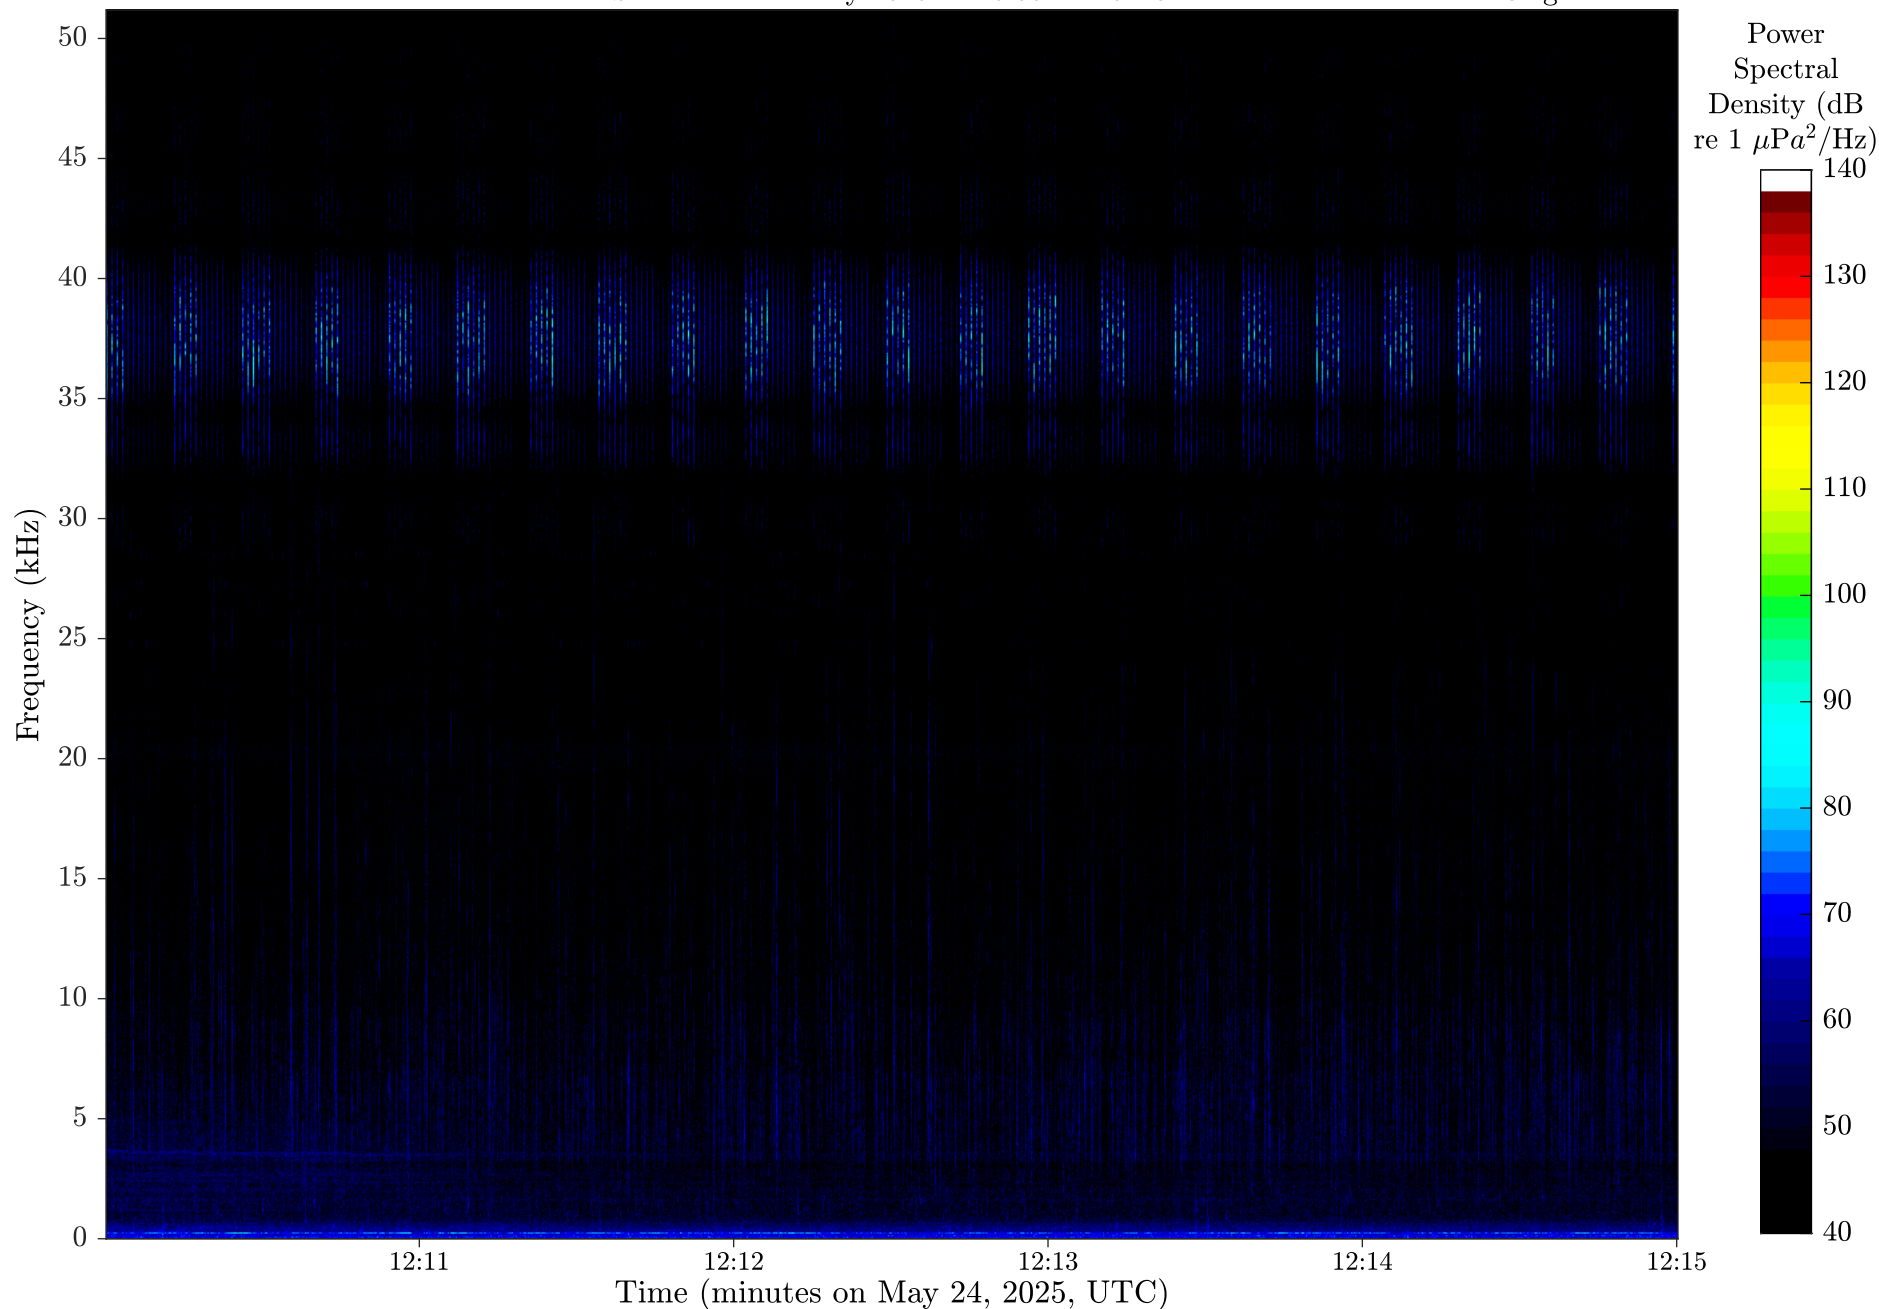


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:02 UTC

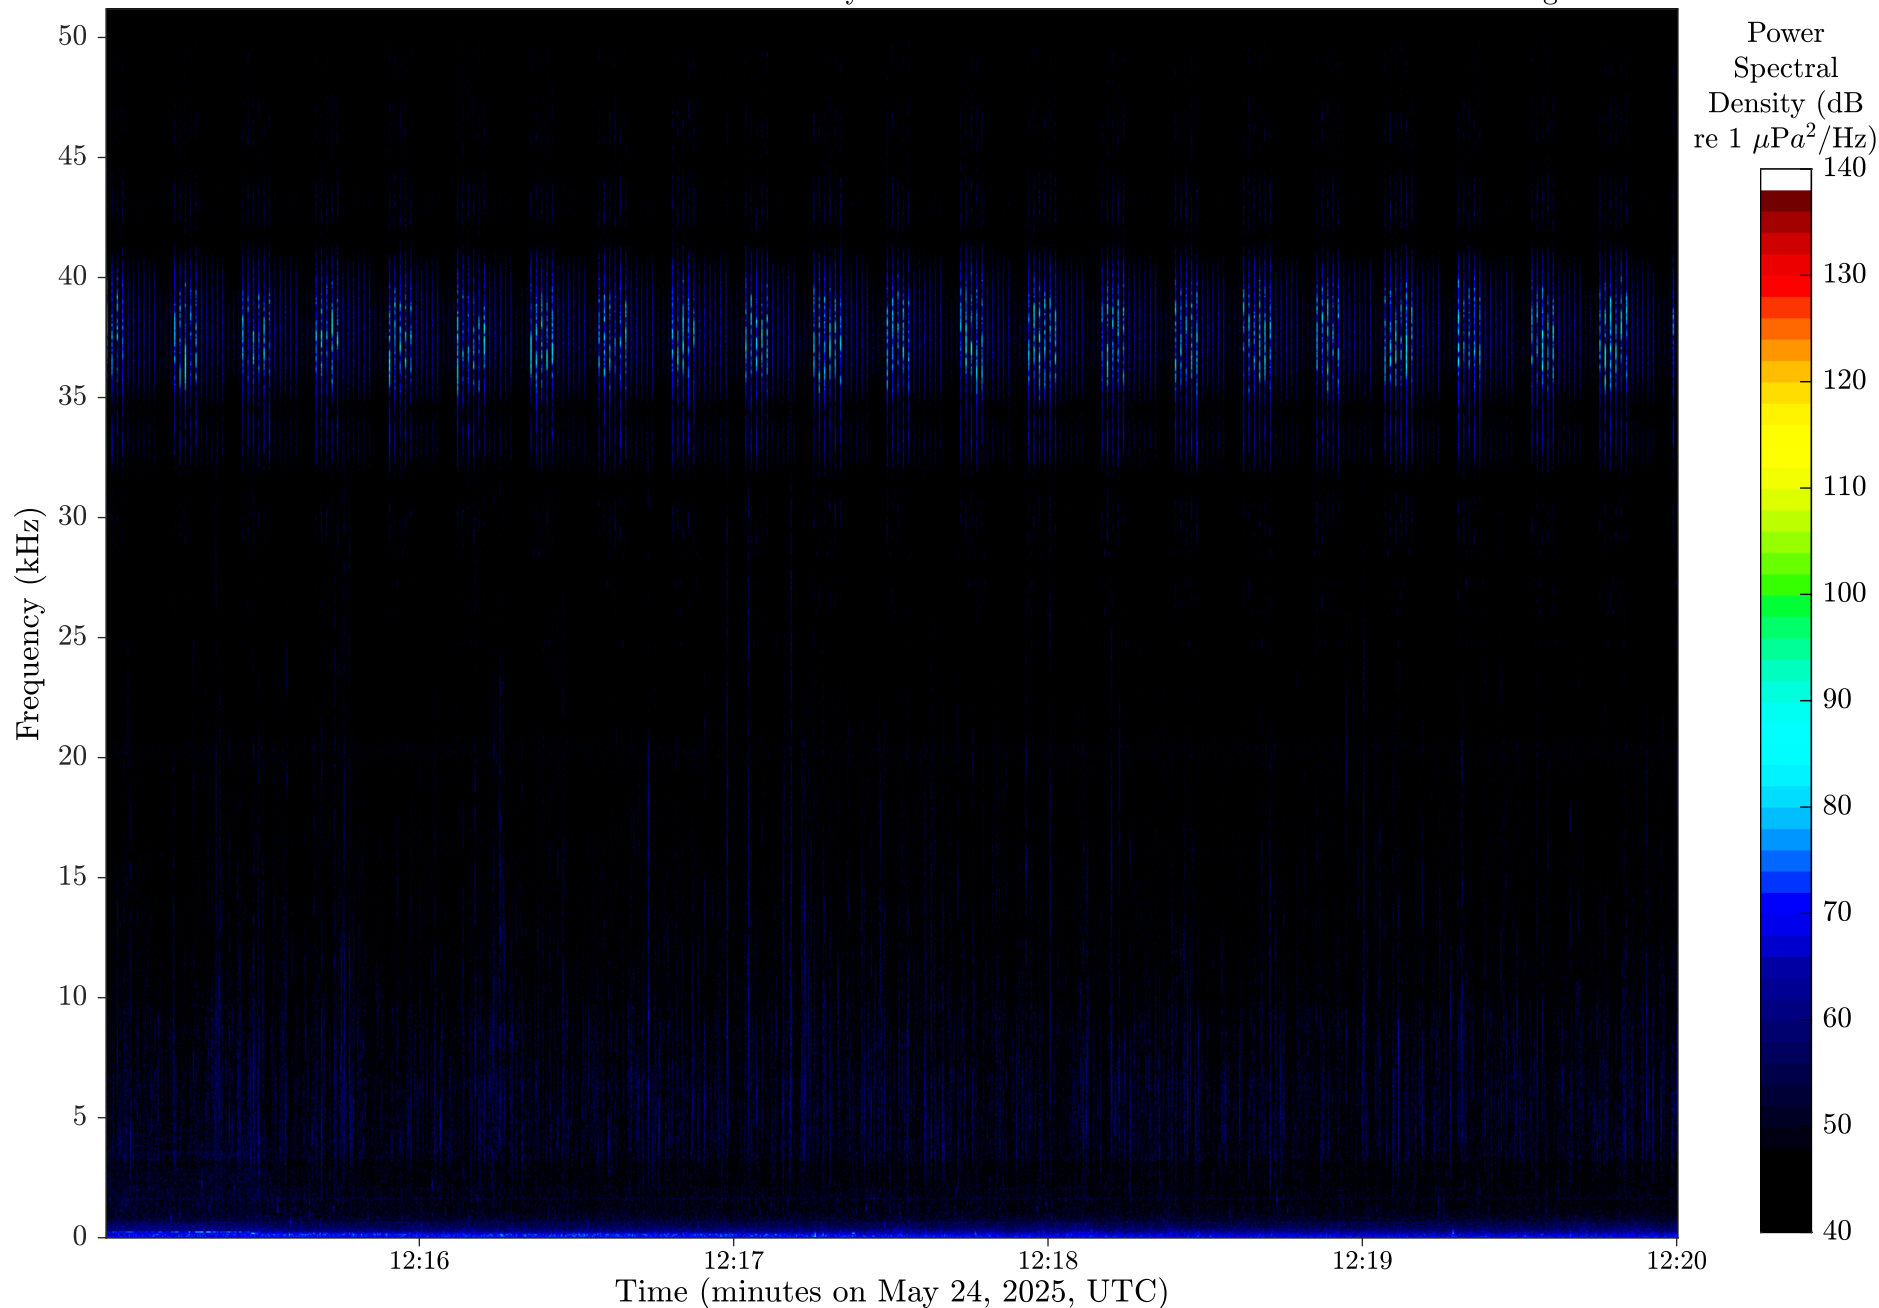


Comments: 32.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:39:10 UTC

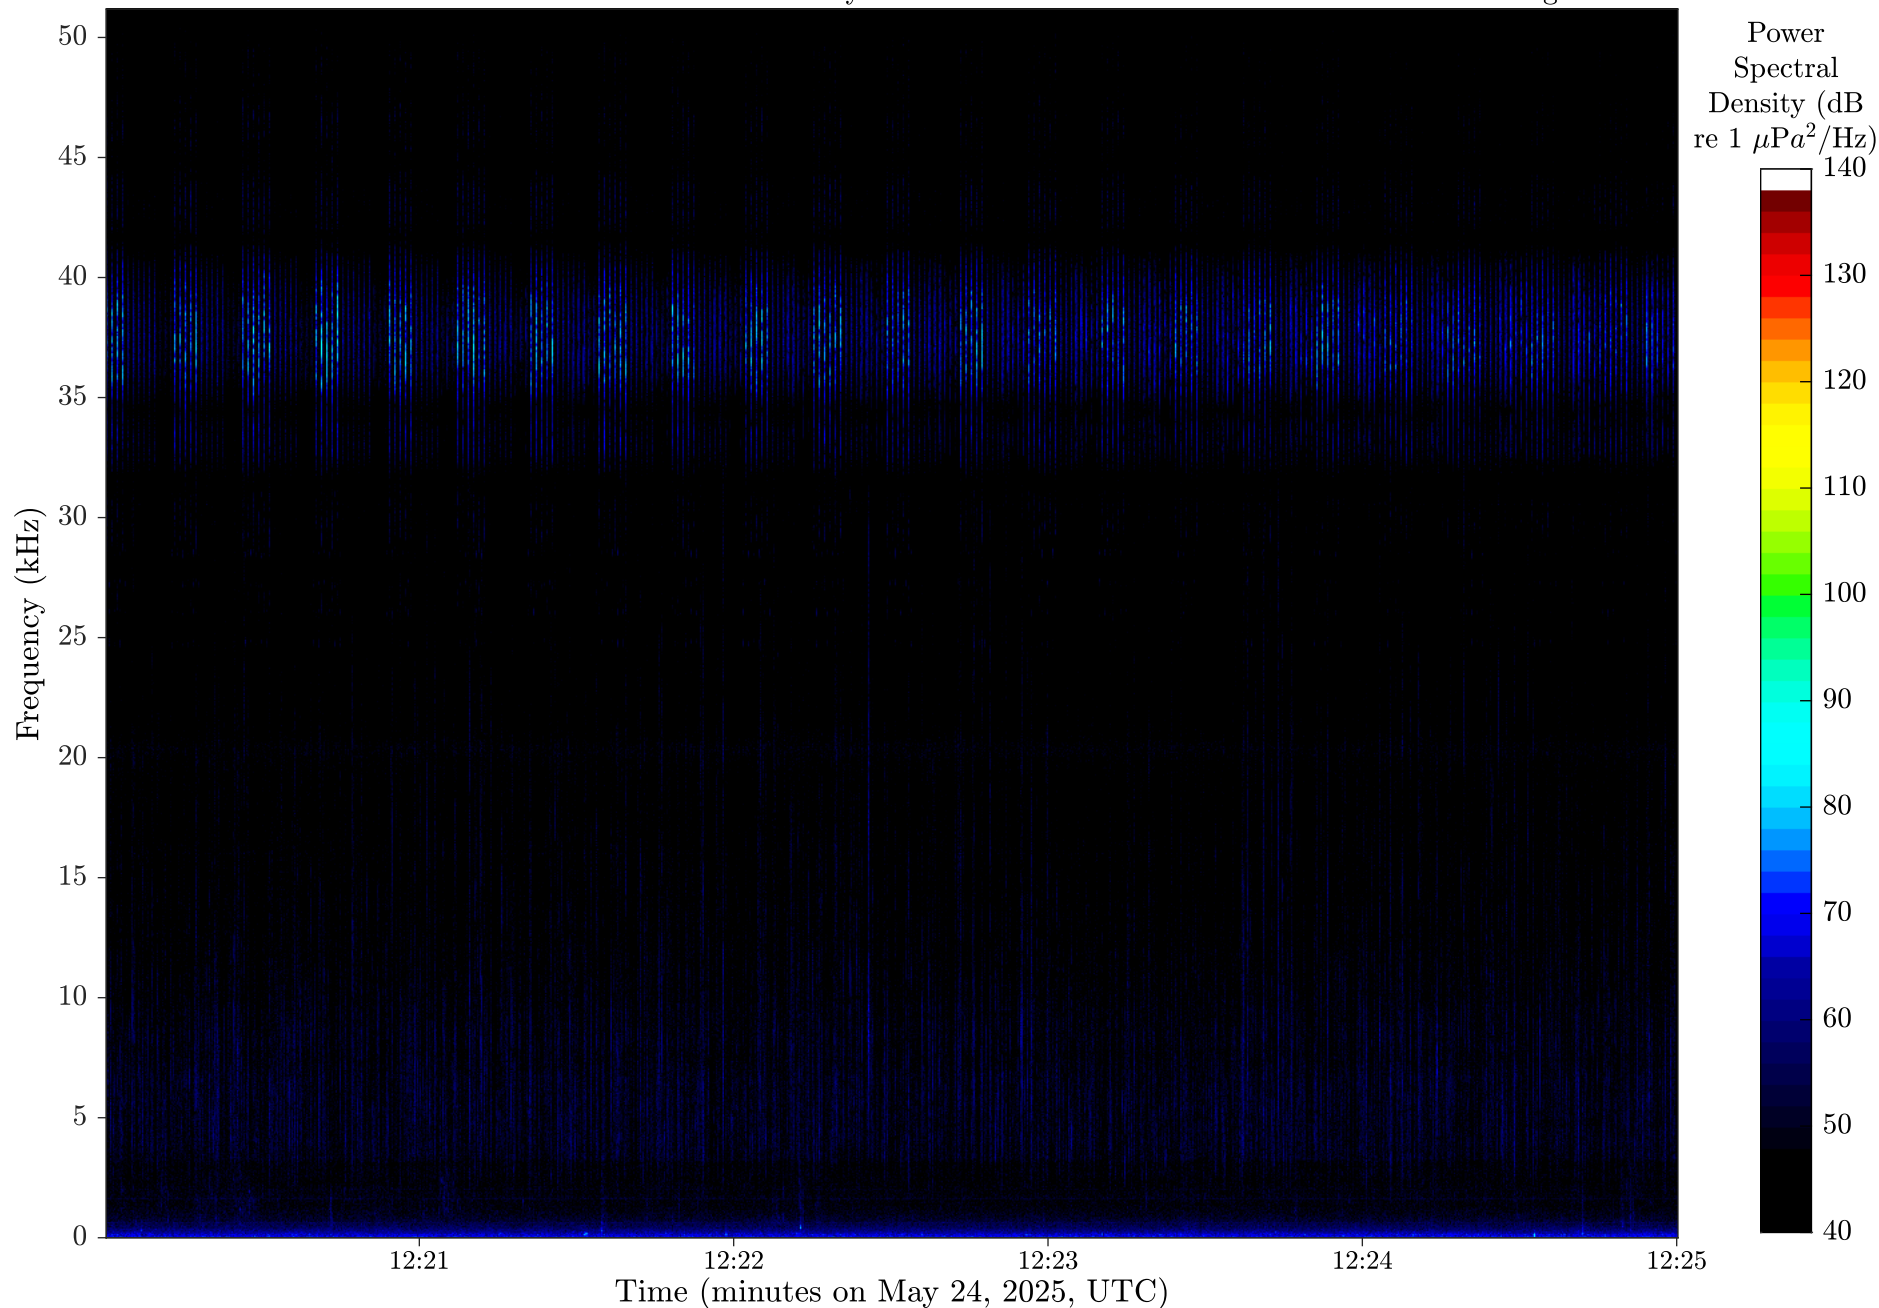

Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:39:18 UTC

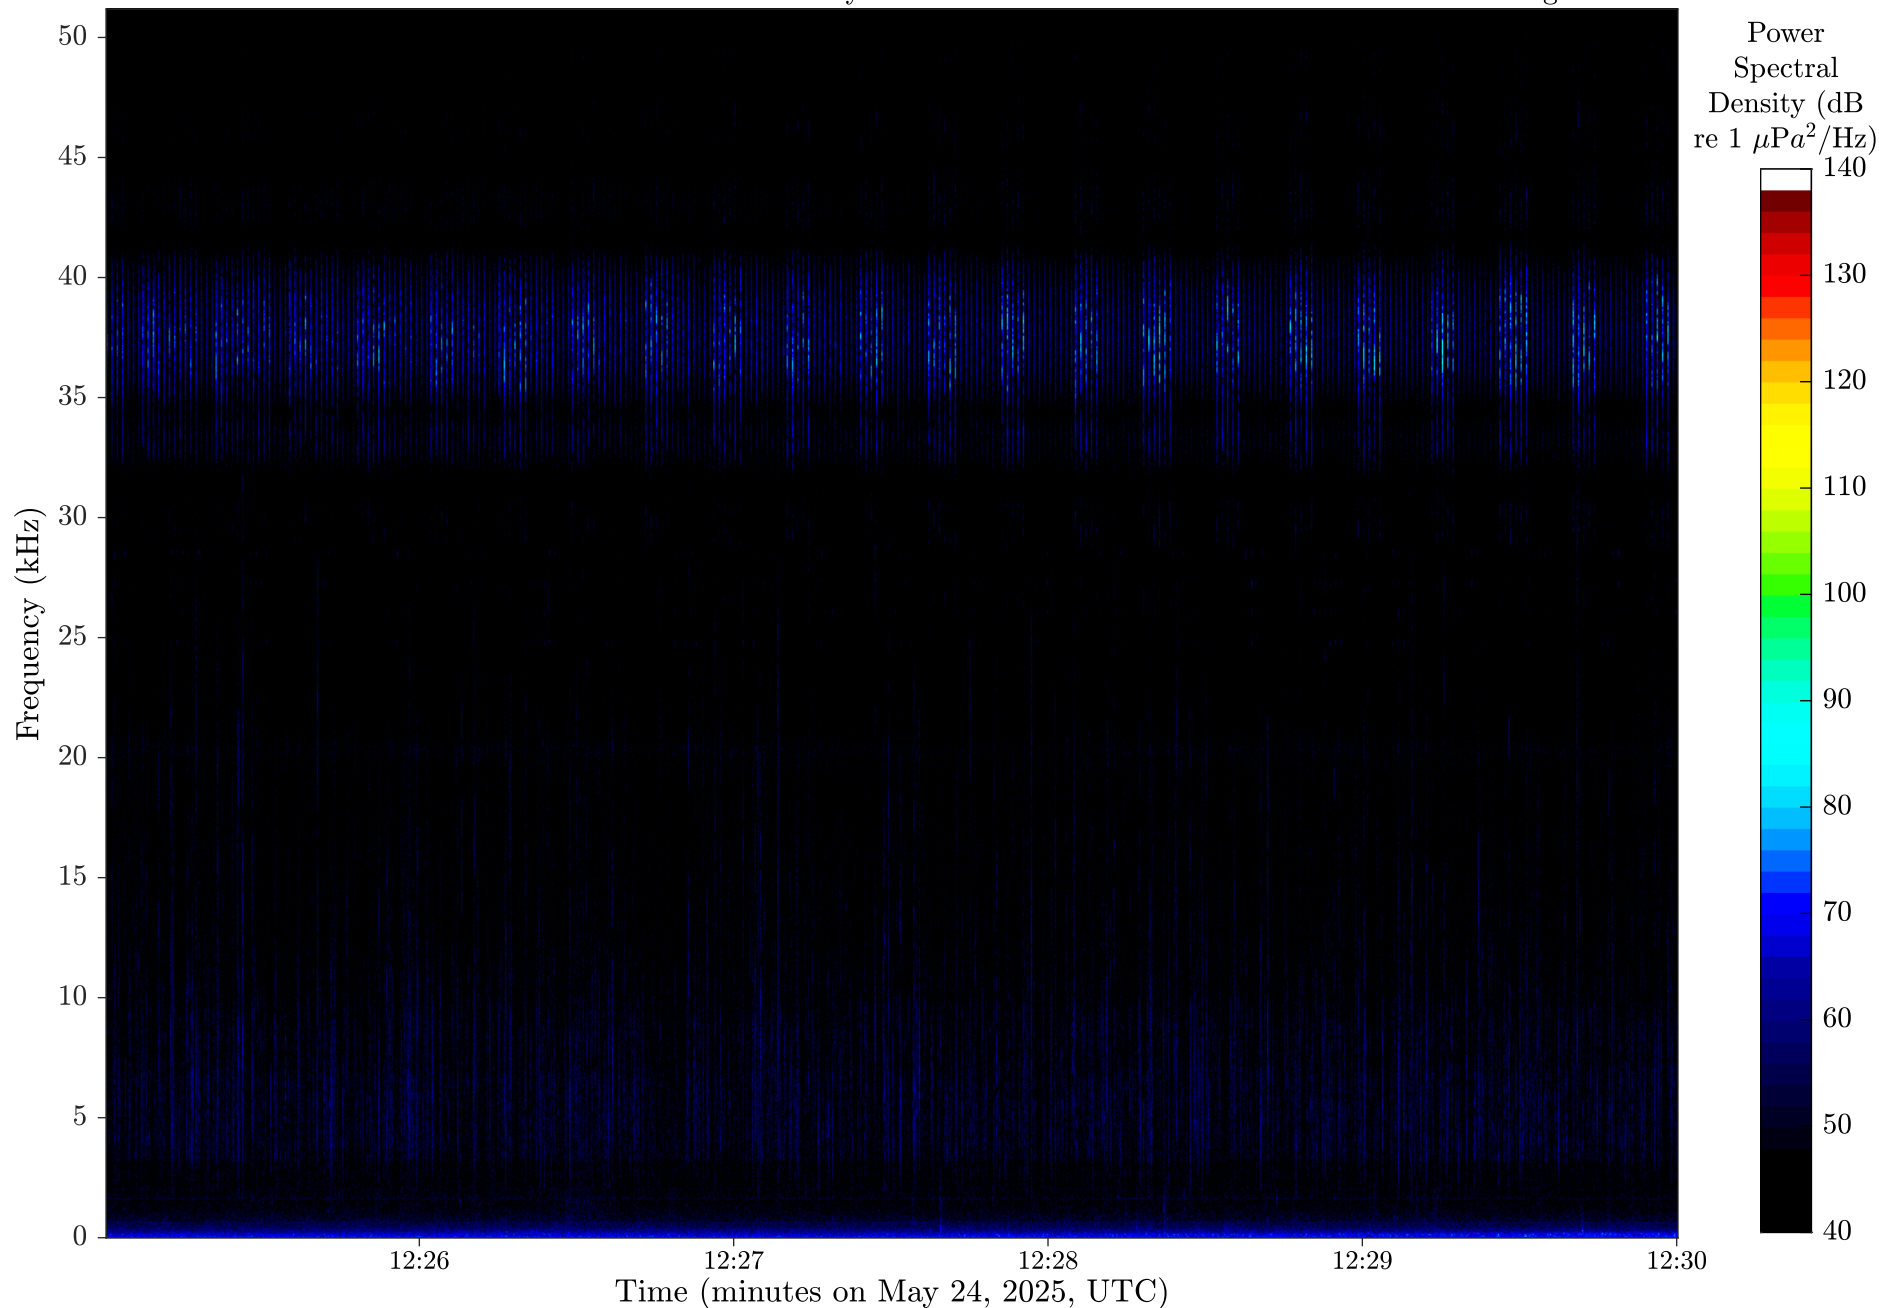

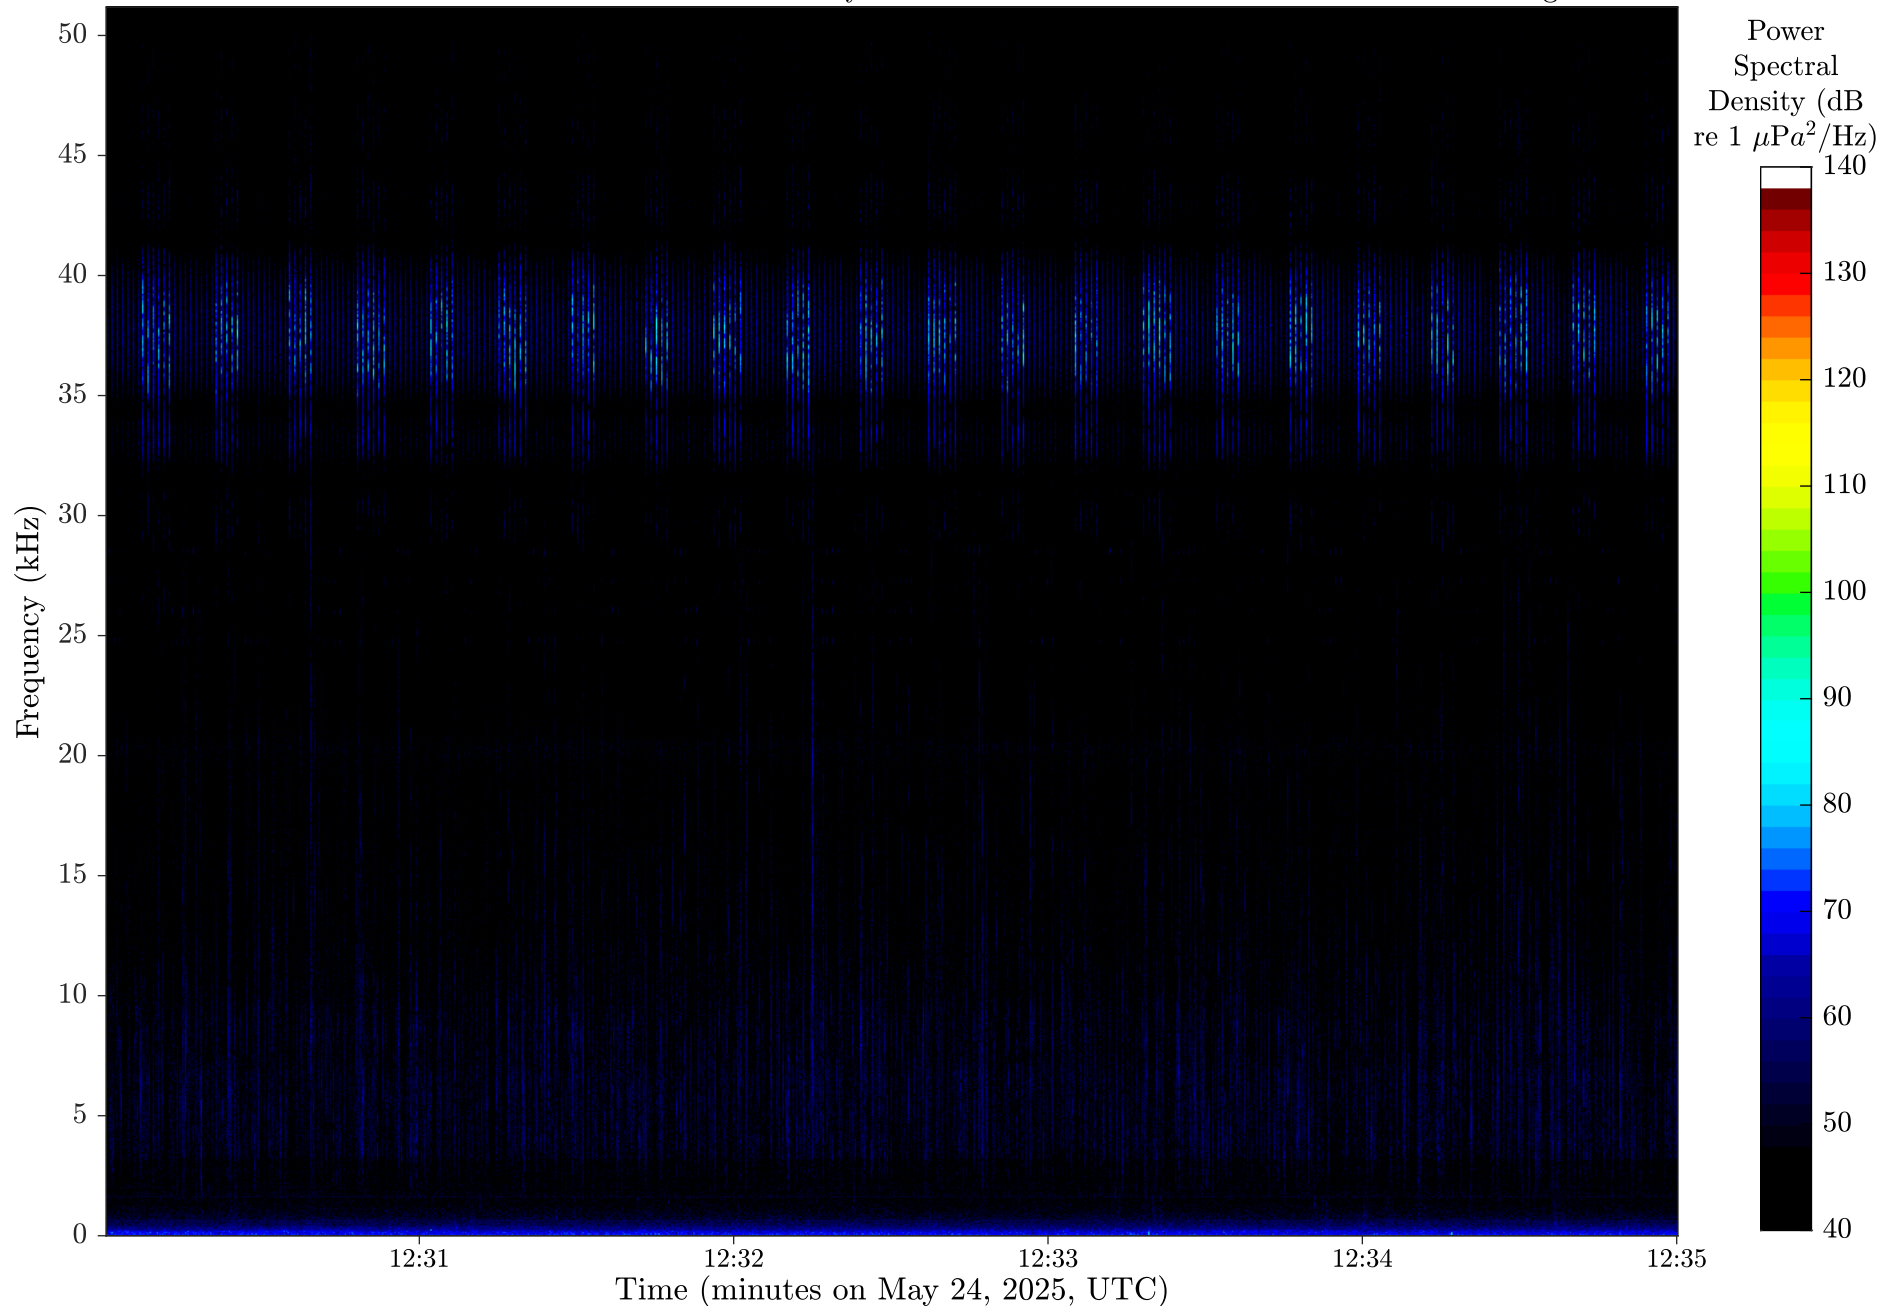


Comments: 31.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:34 UTC

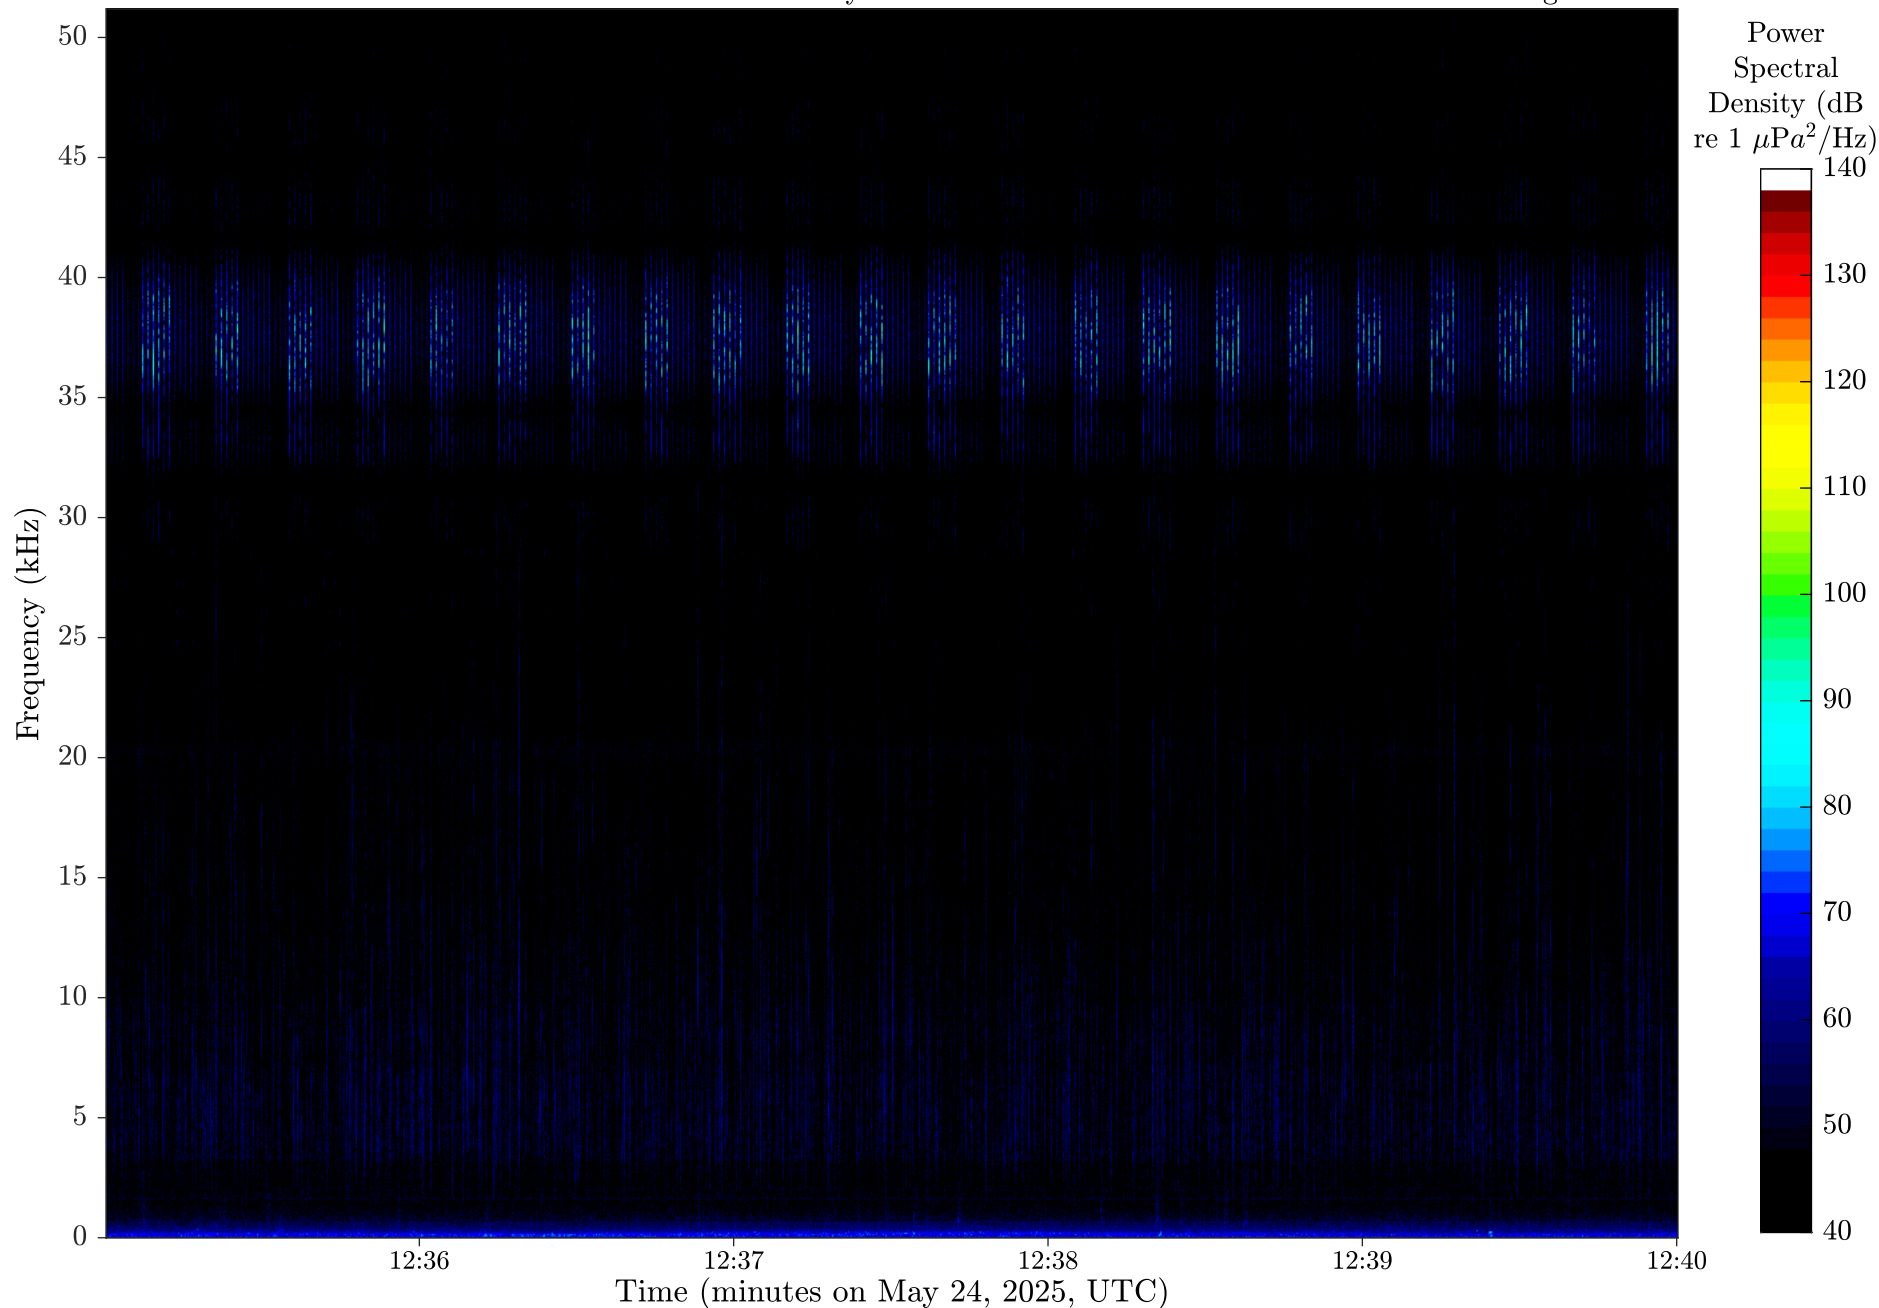


Comments: 32.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:42 UTC

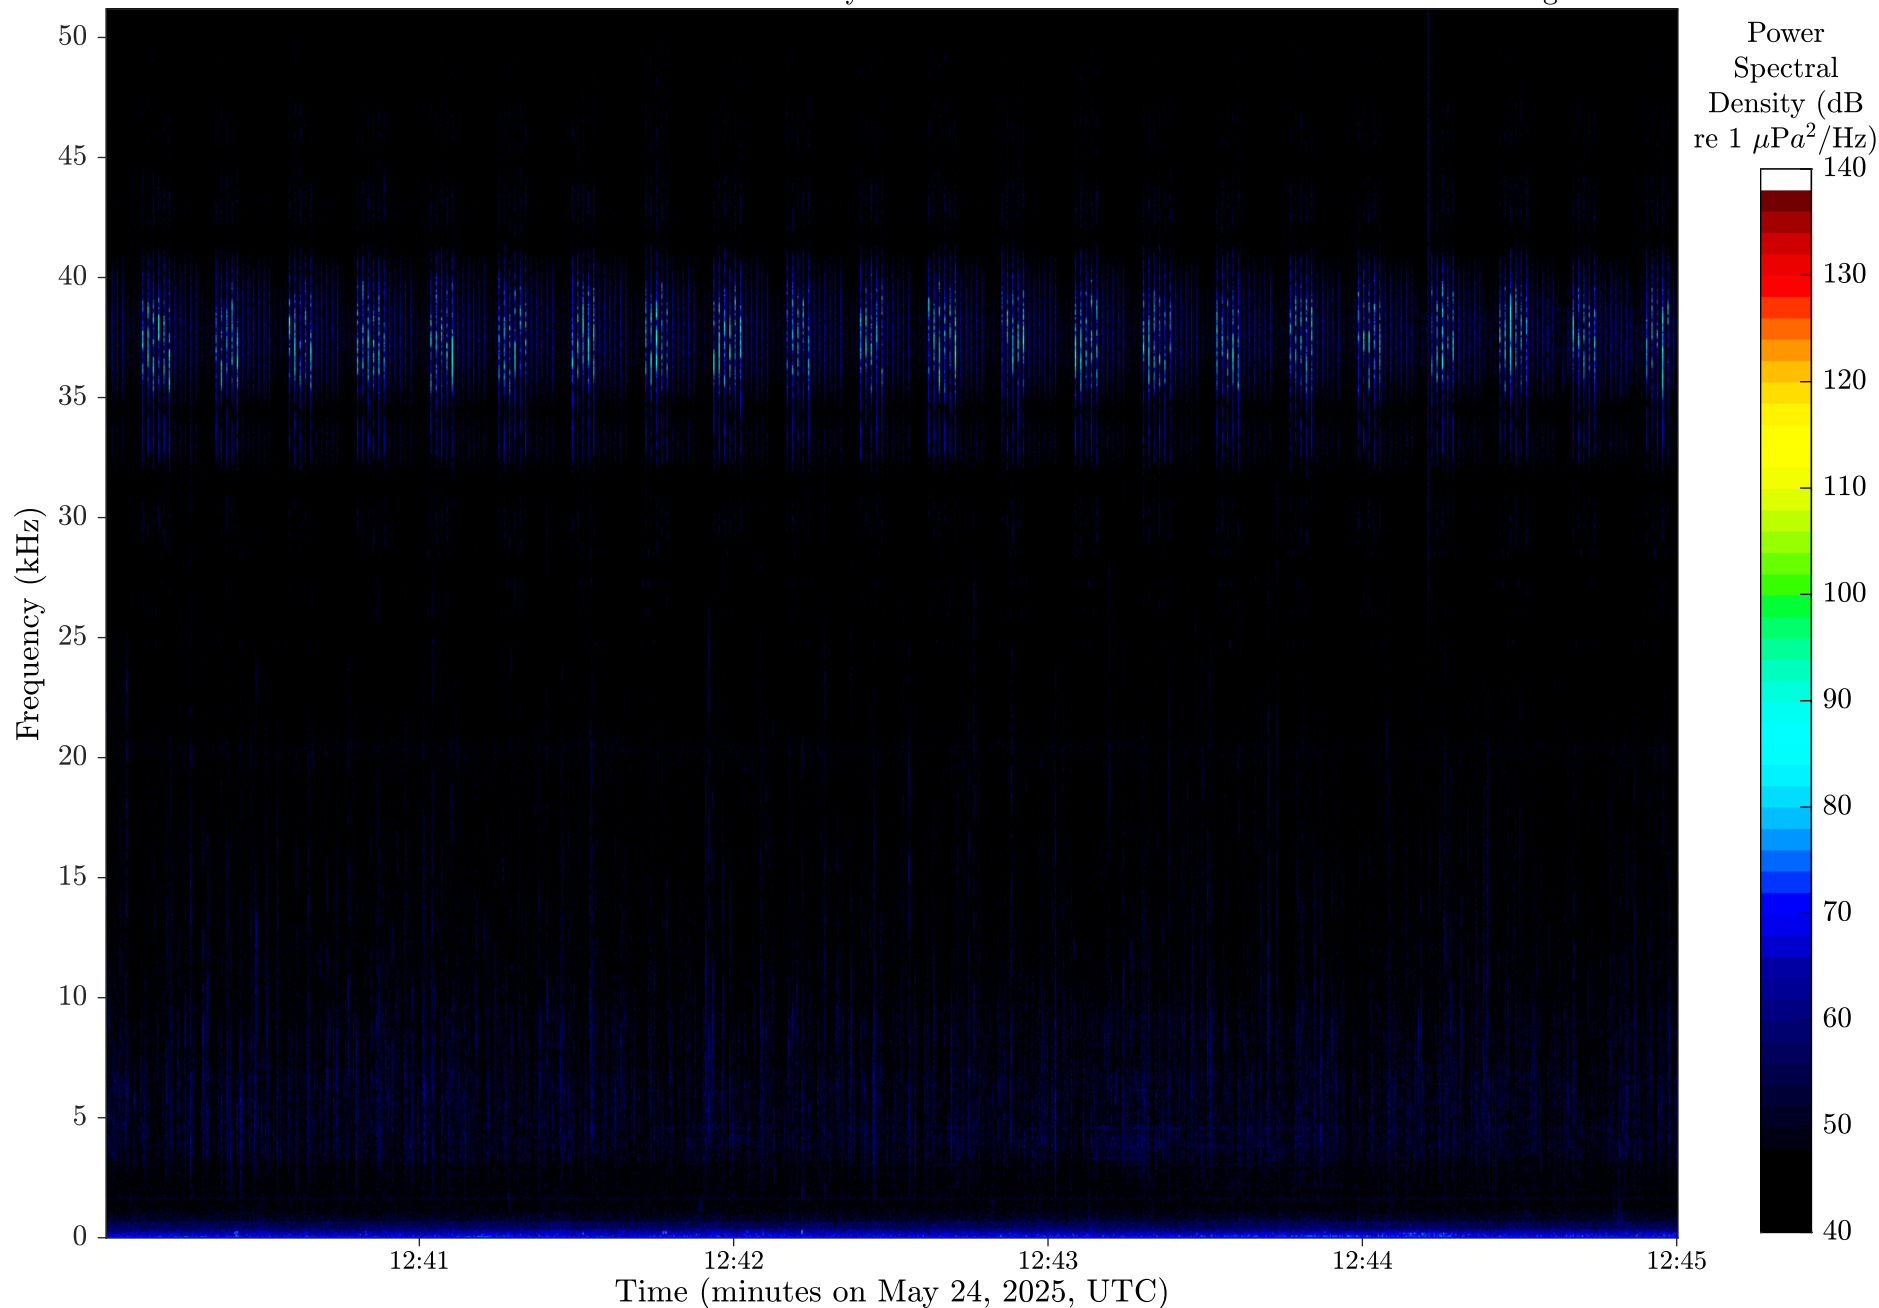


Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:51 UTC

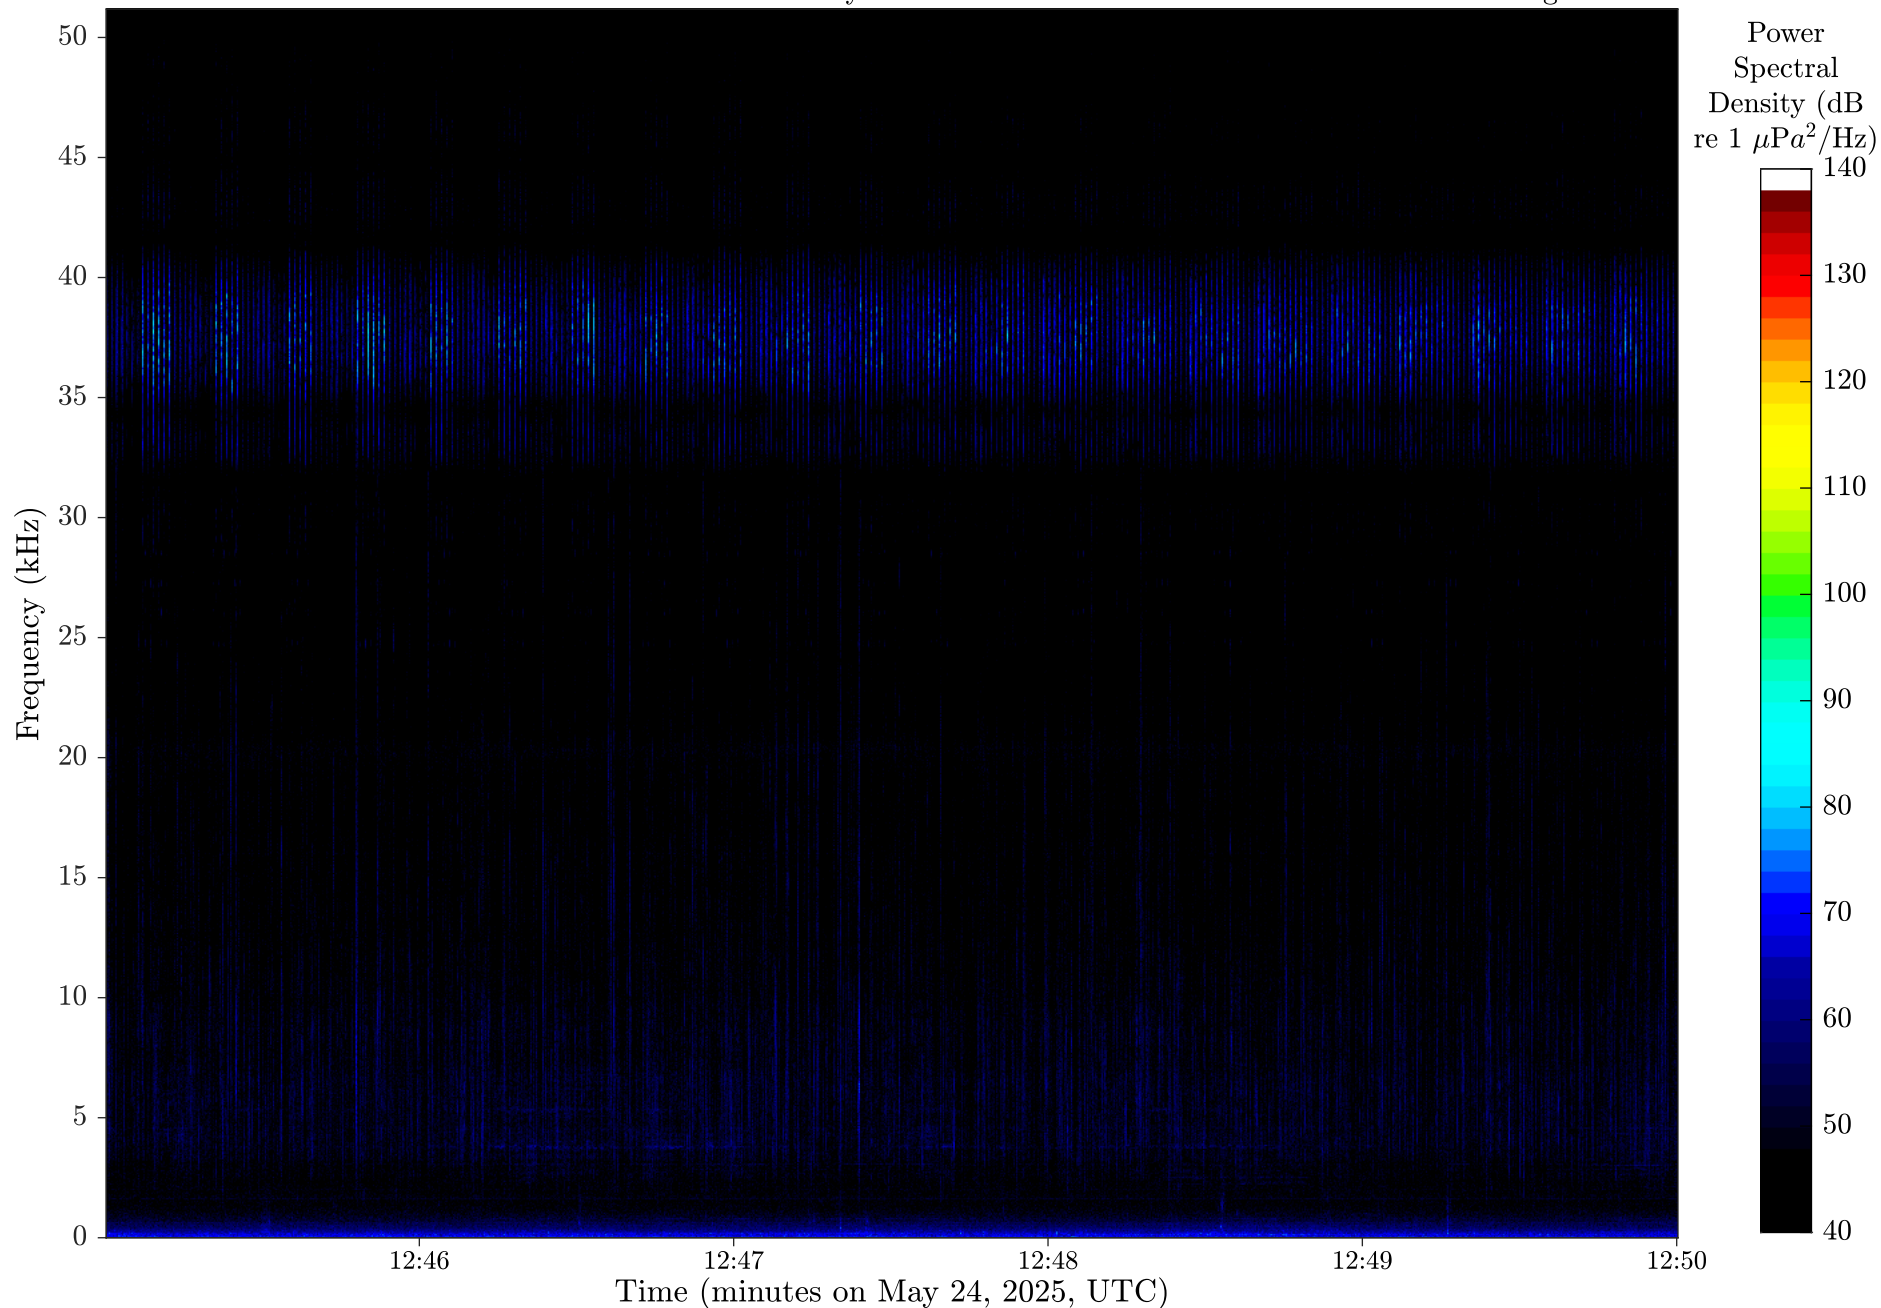


Comments: 30.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:39:59 UTC

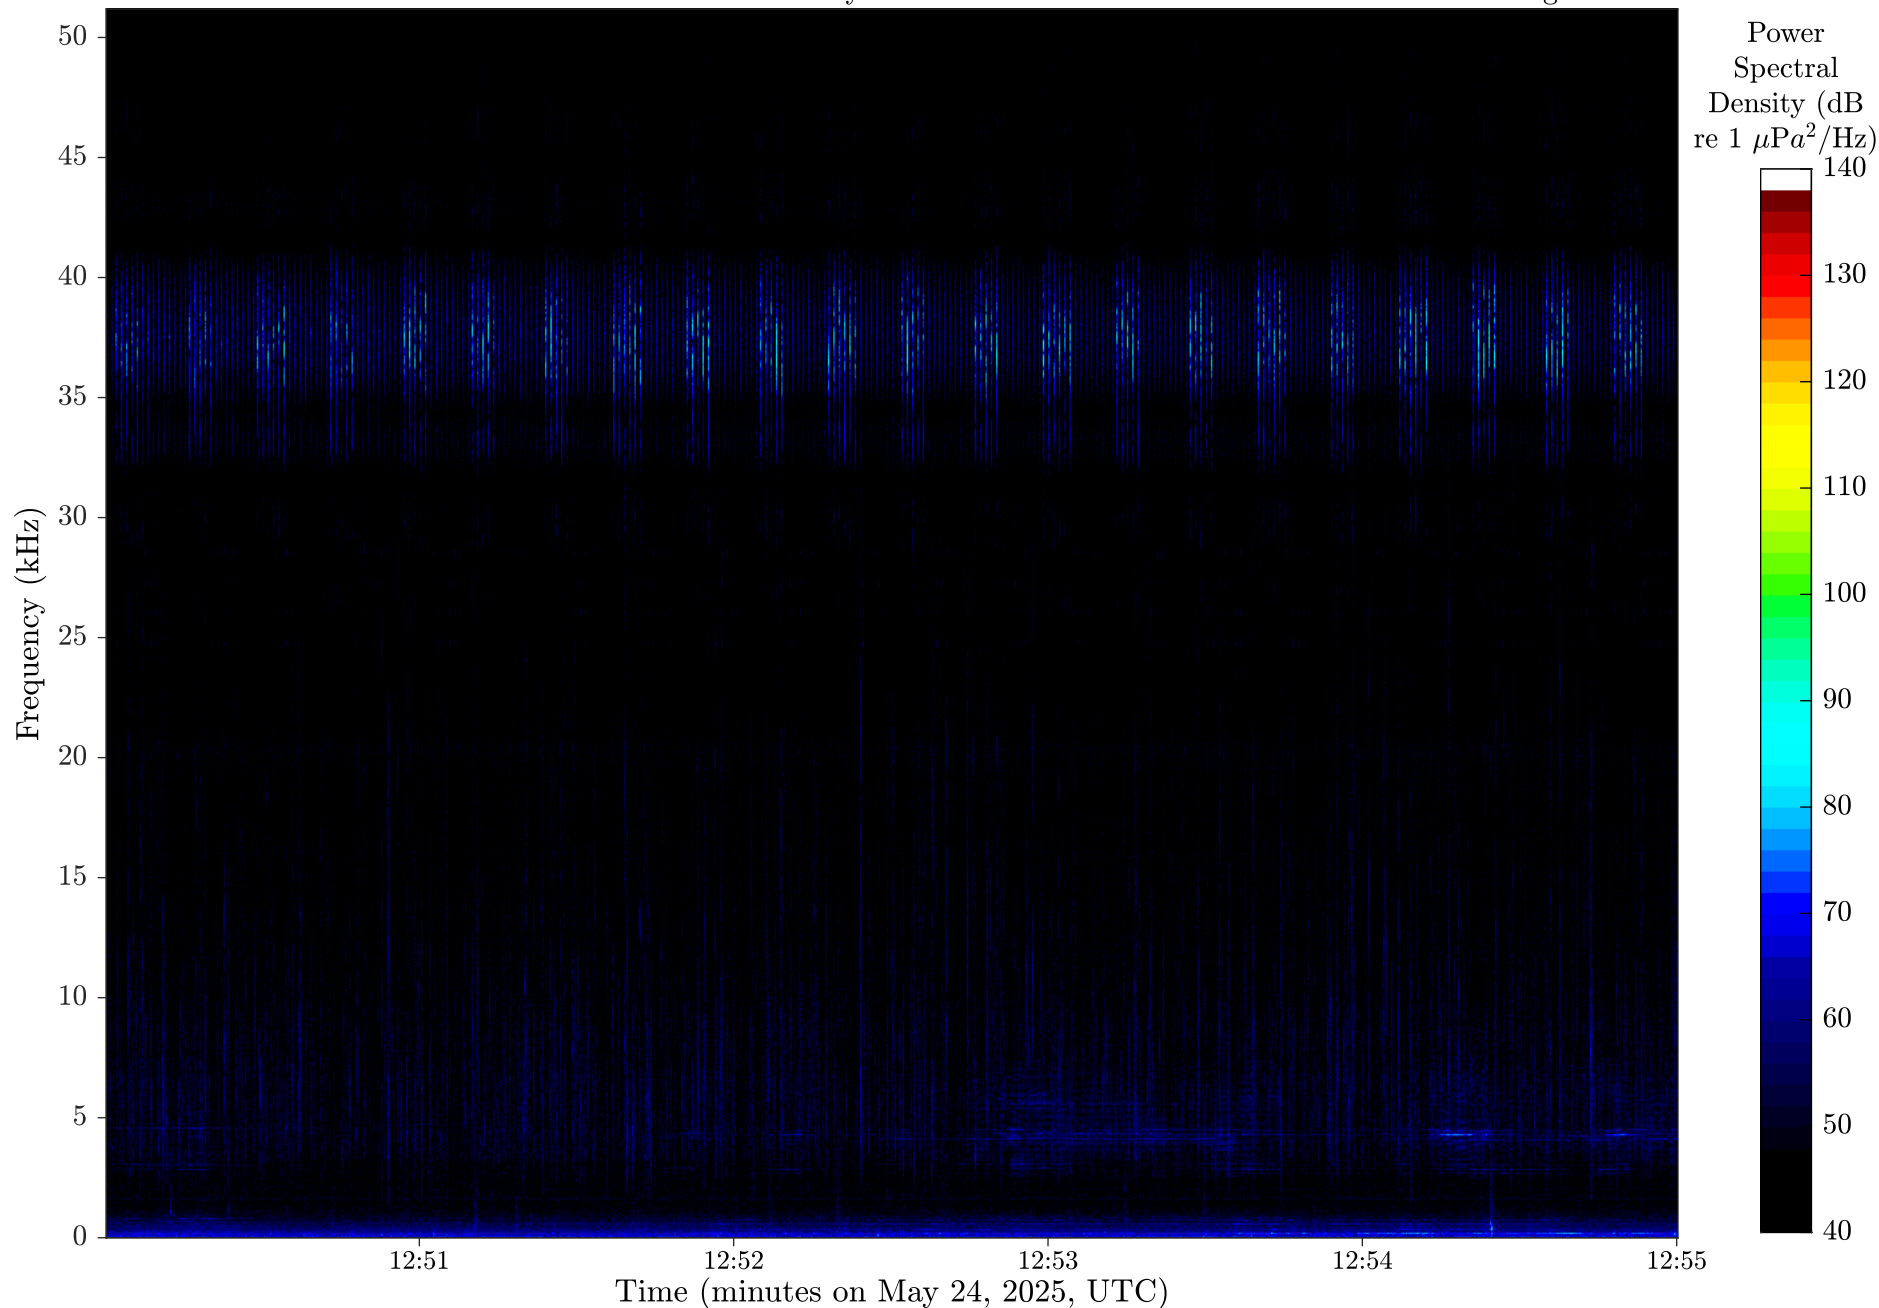


Comments: 31.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:07 UTC

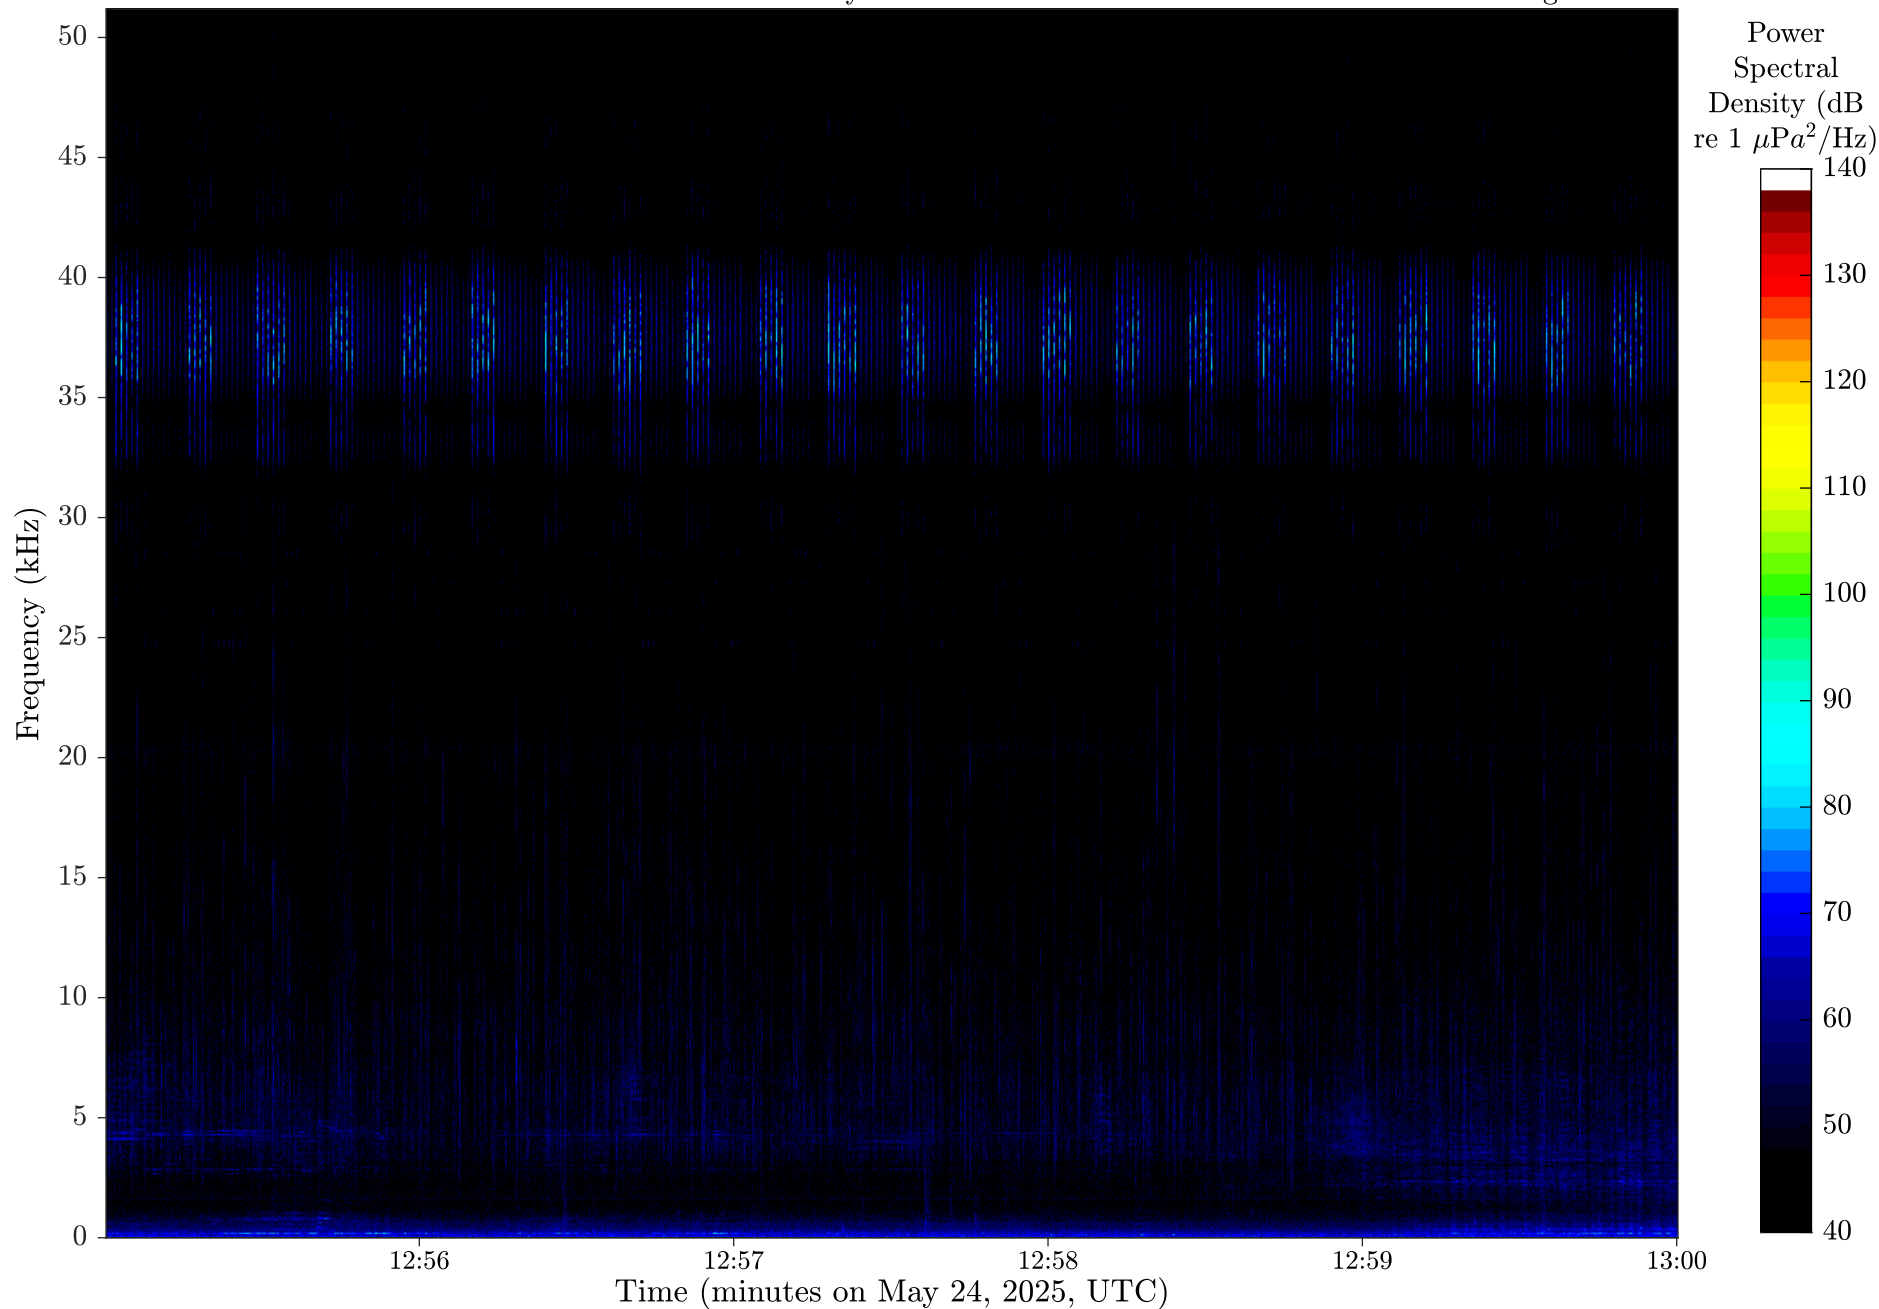


Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:14 UTC

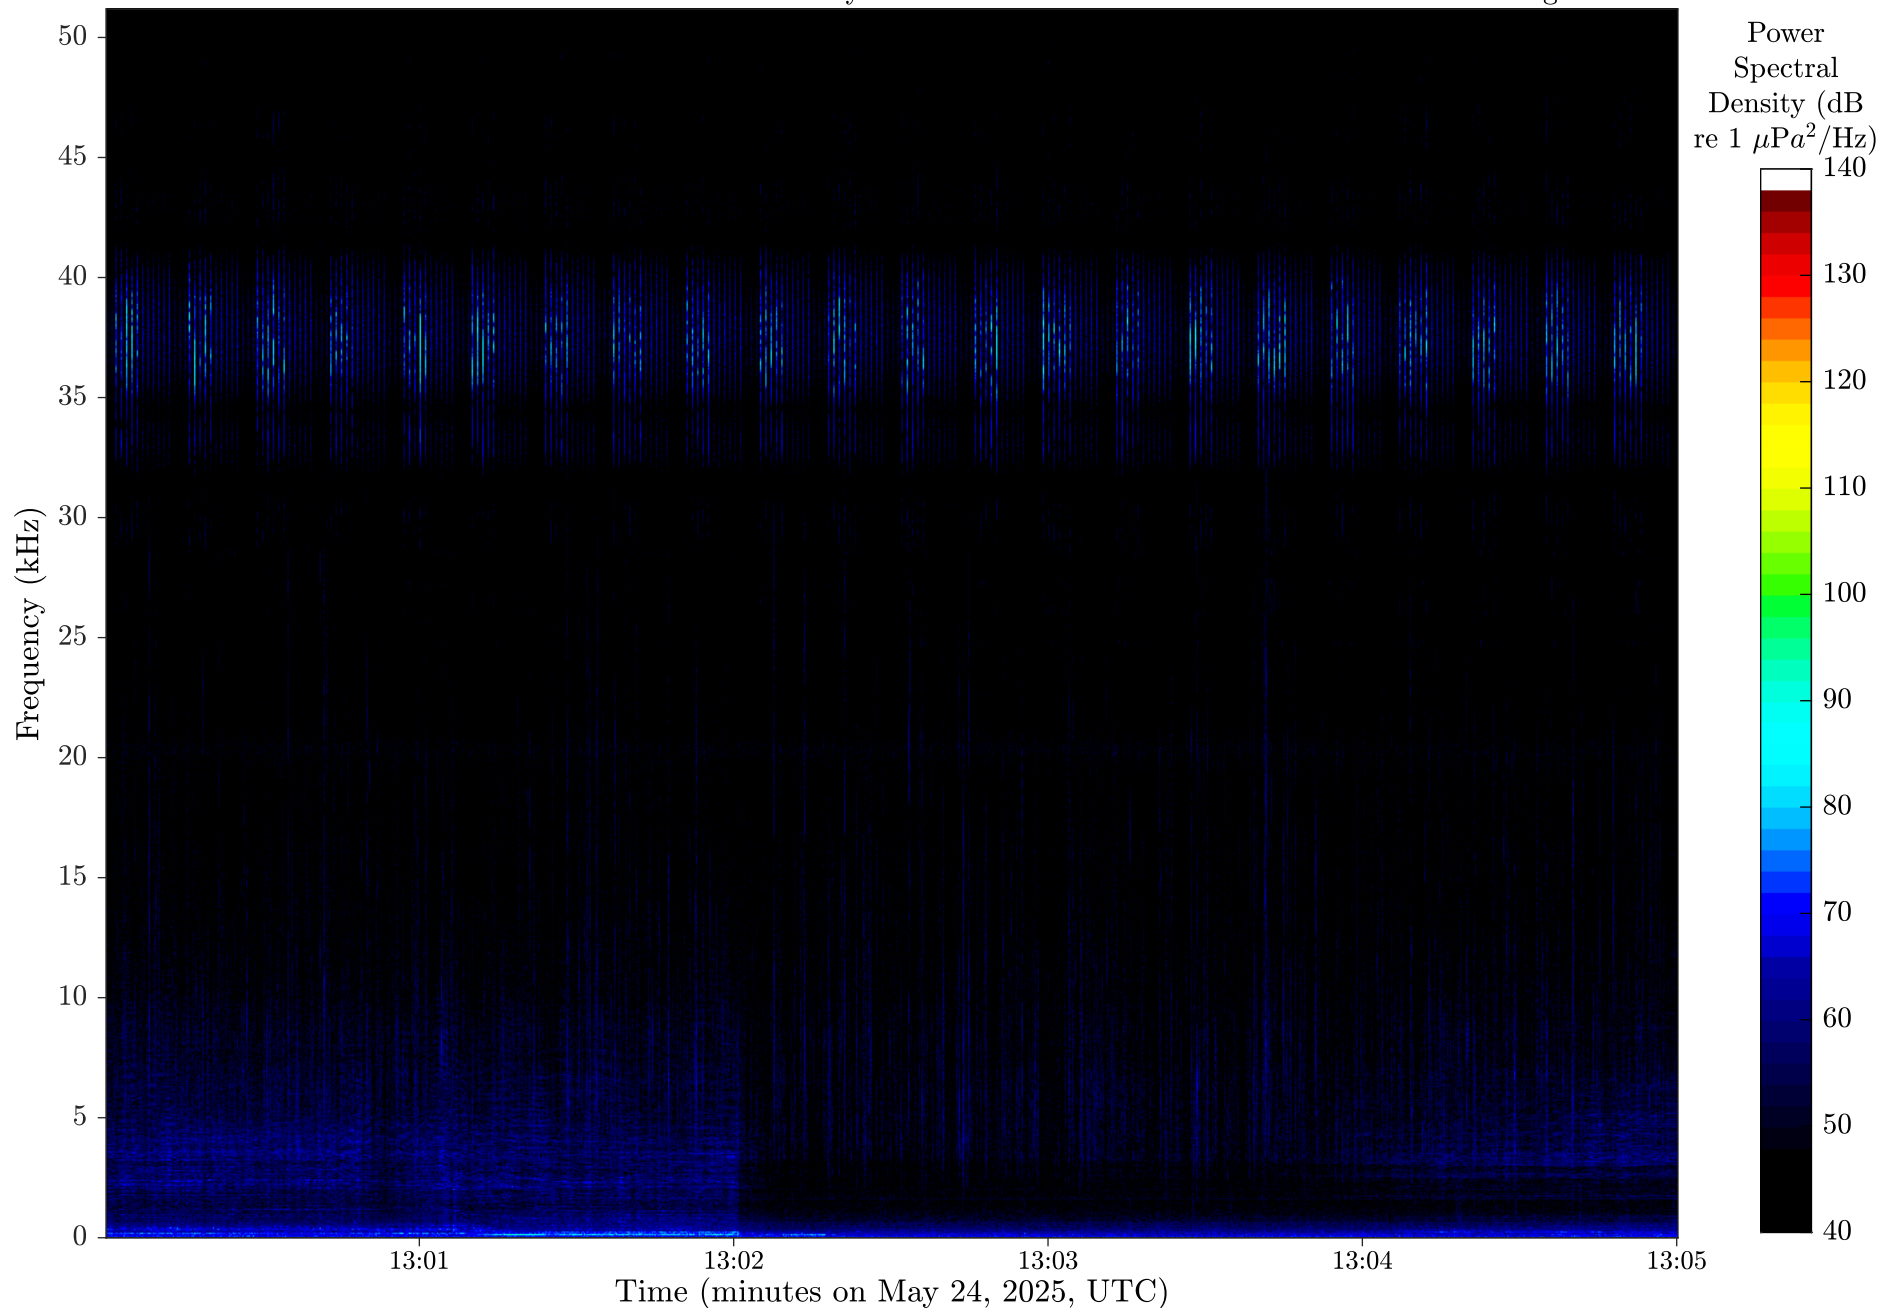


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:40:22 UTC

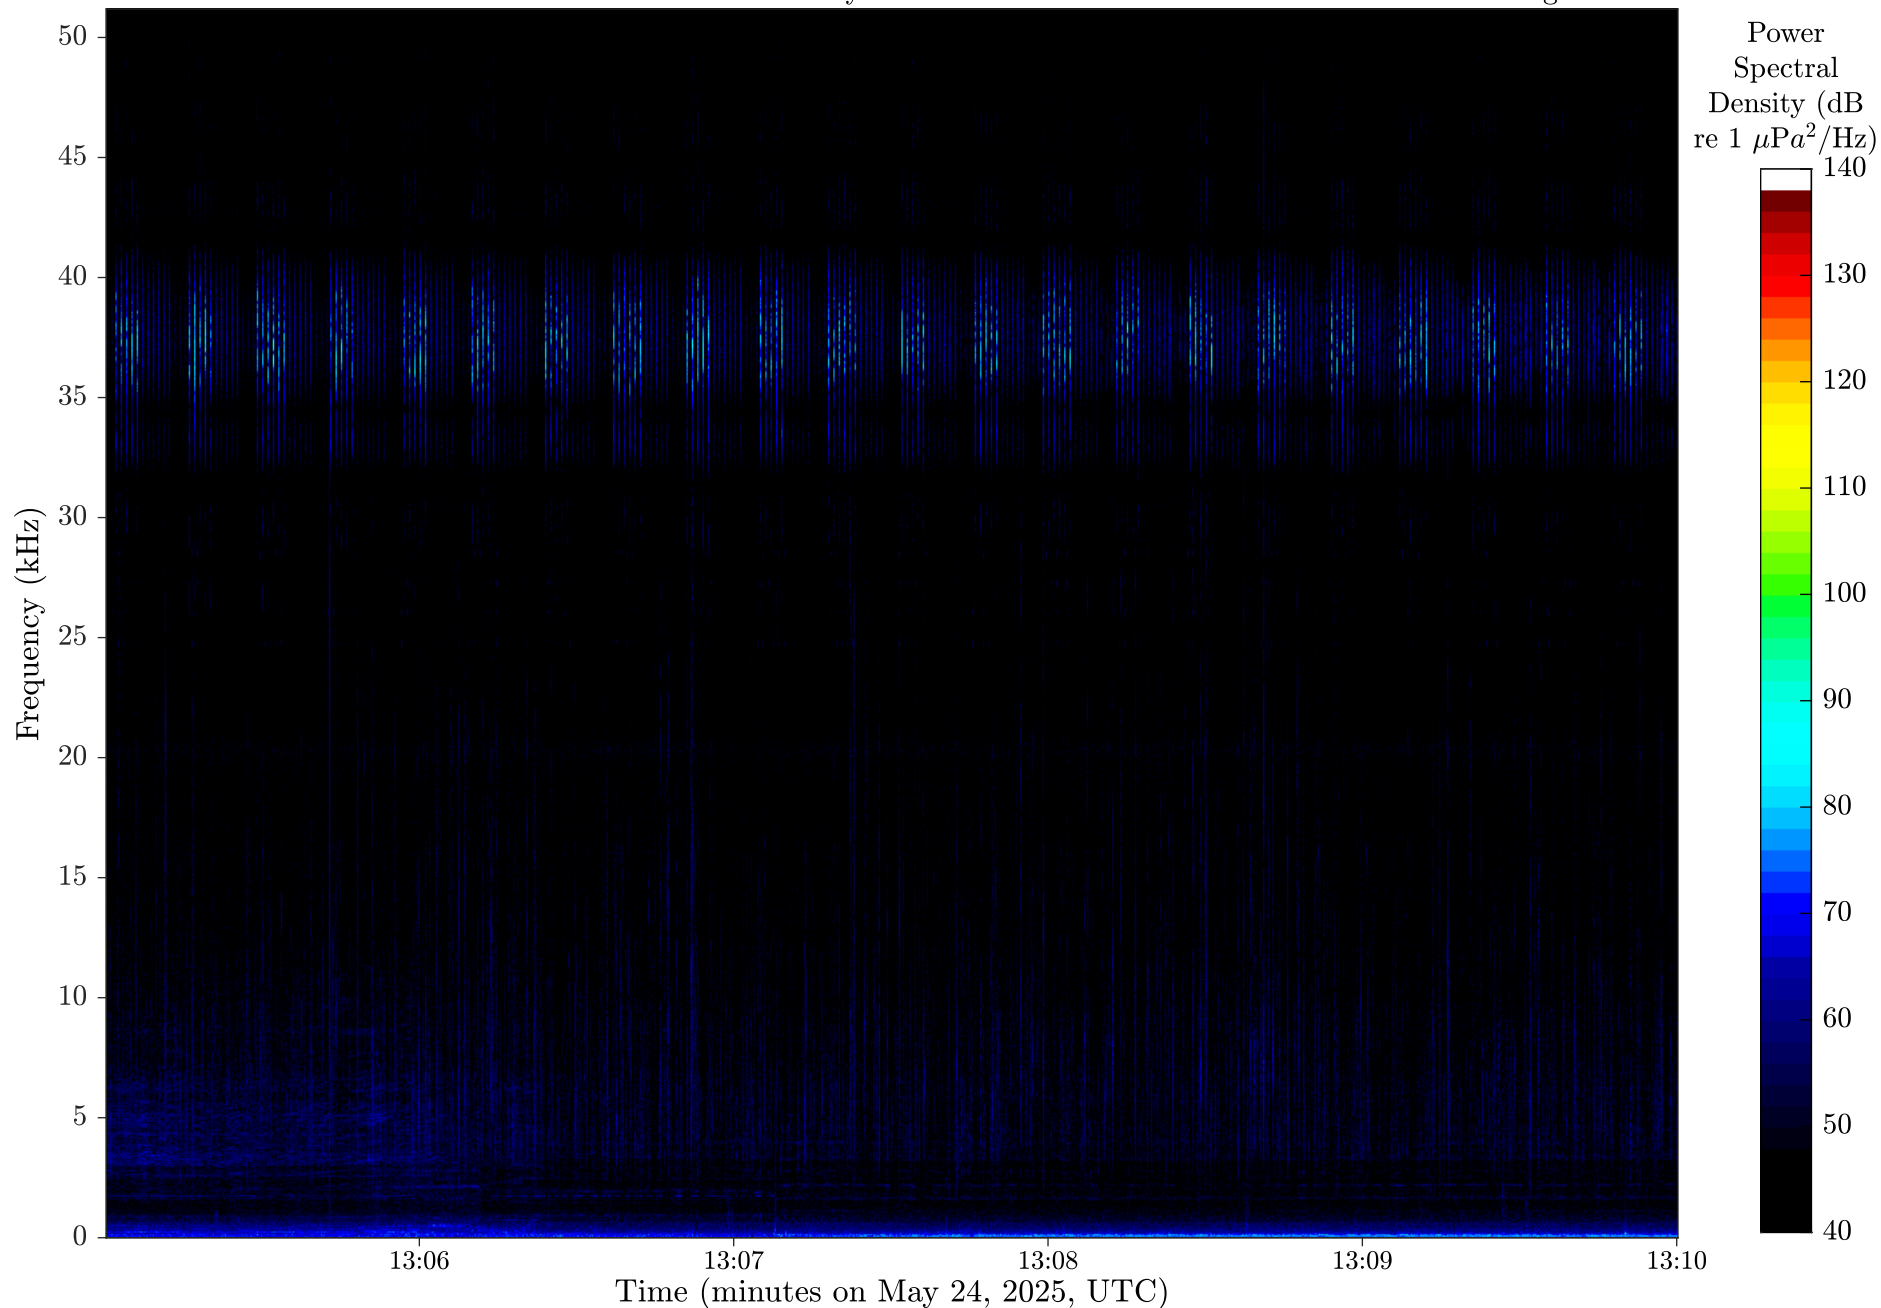


Comments: 31.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:30 UTC

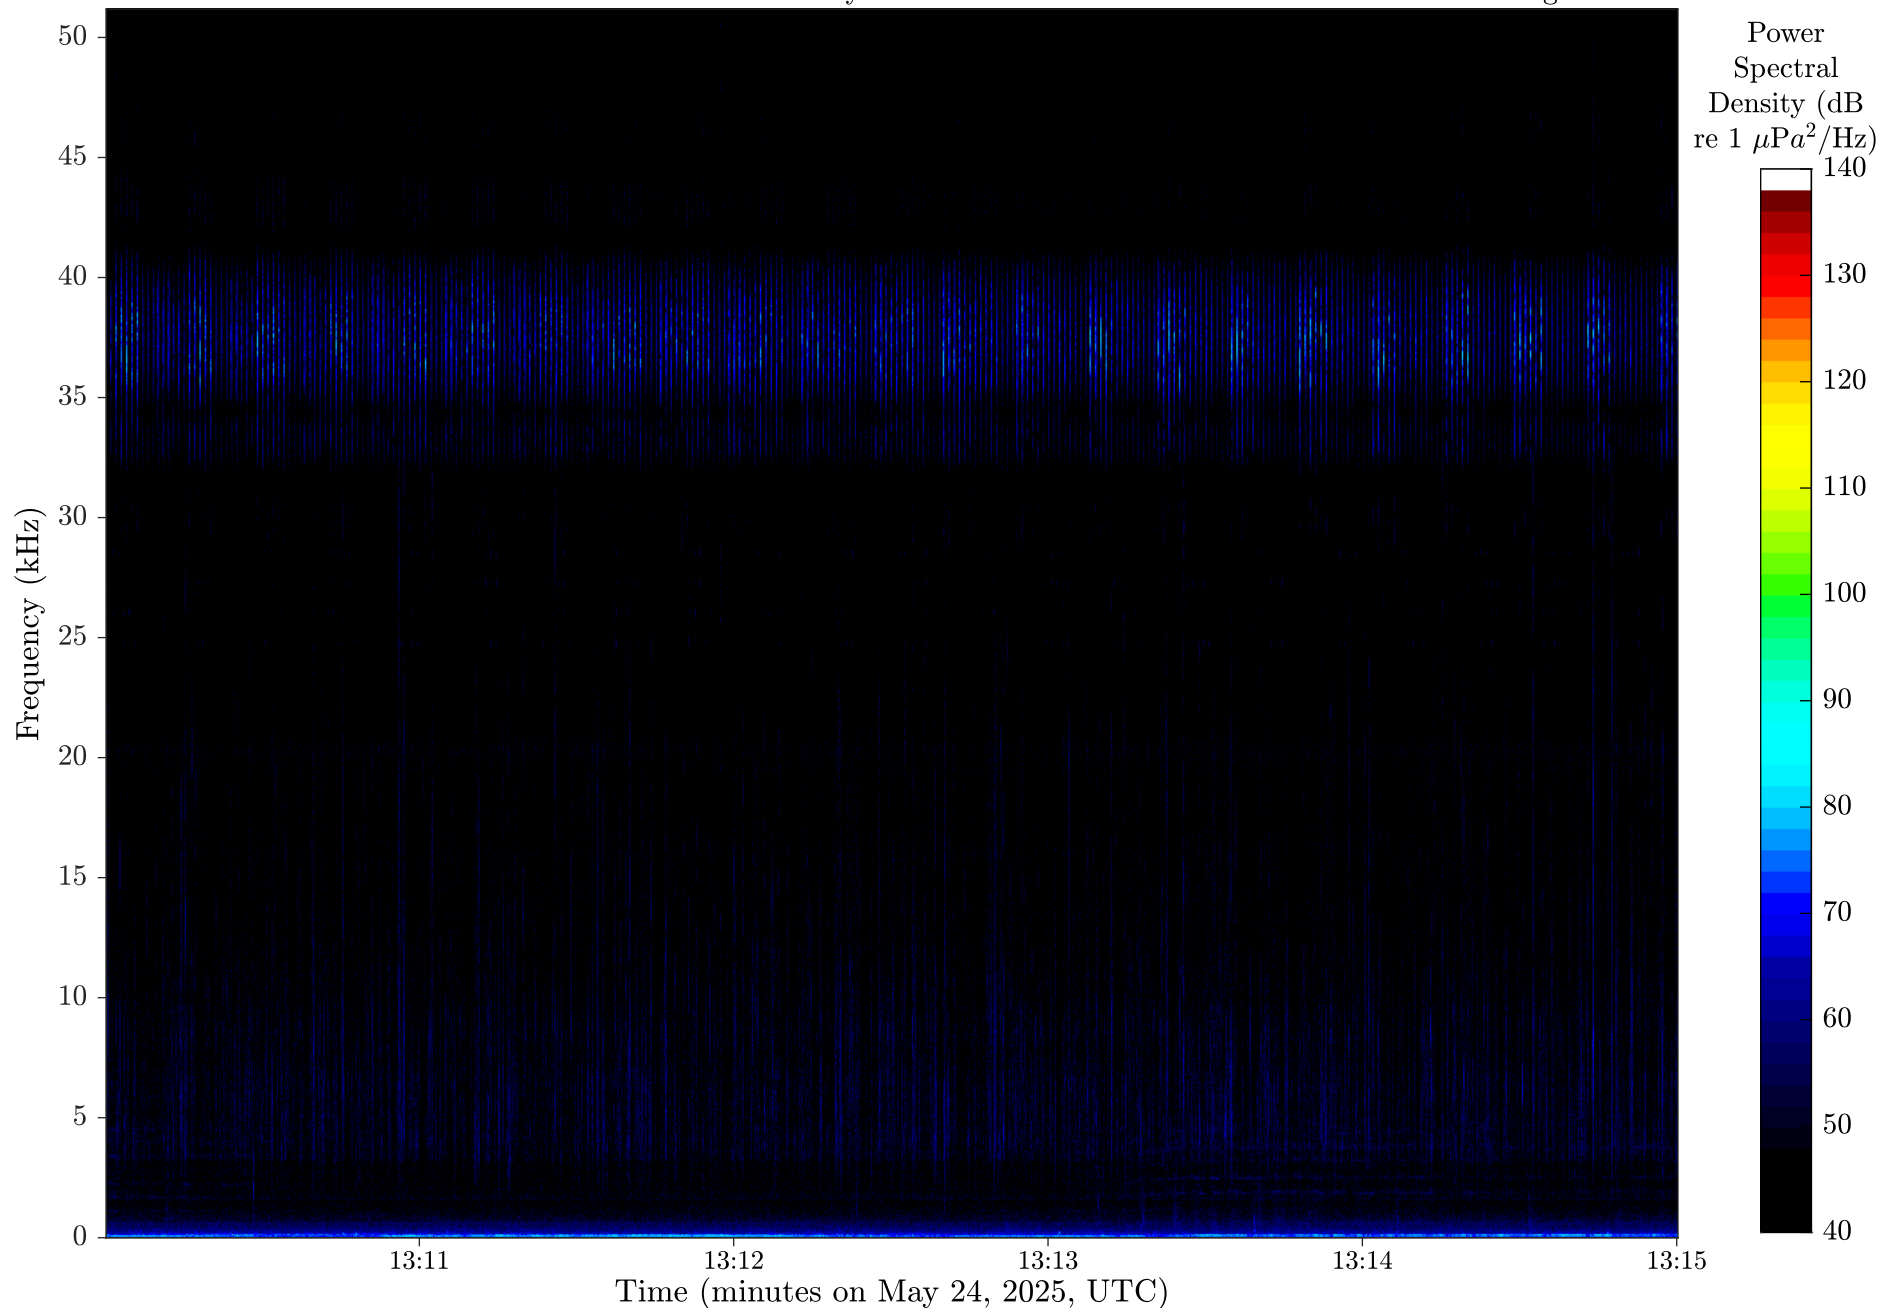


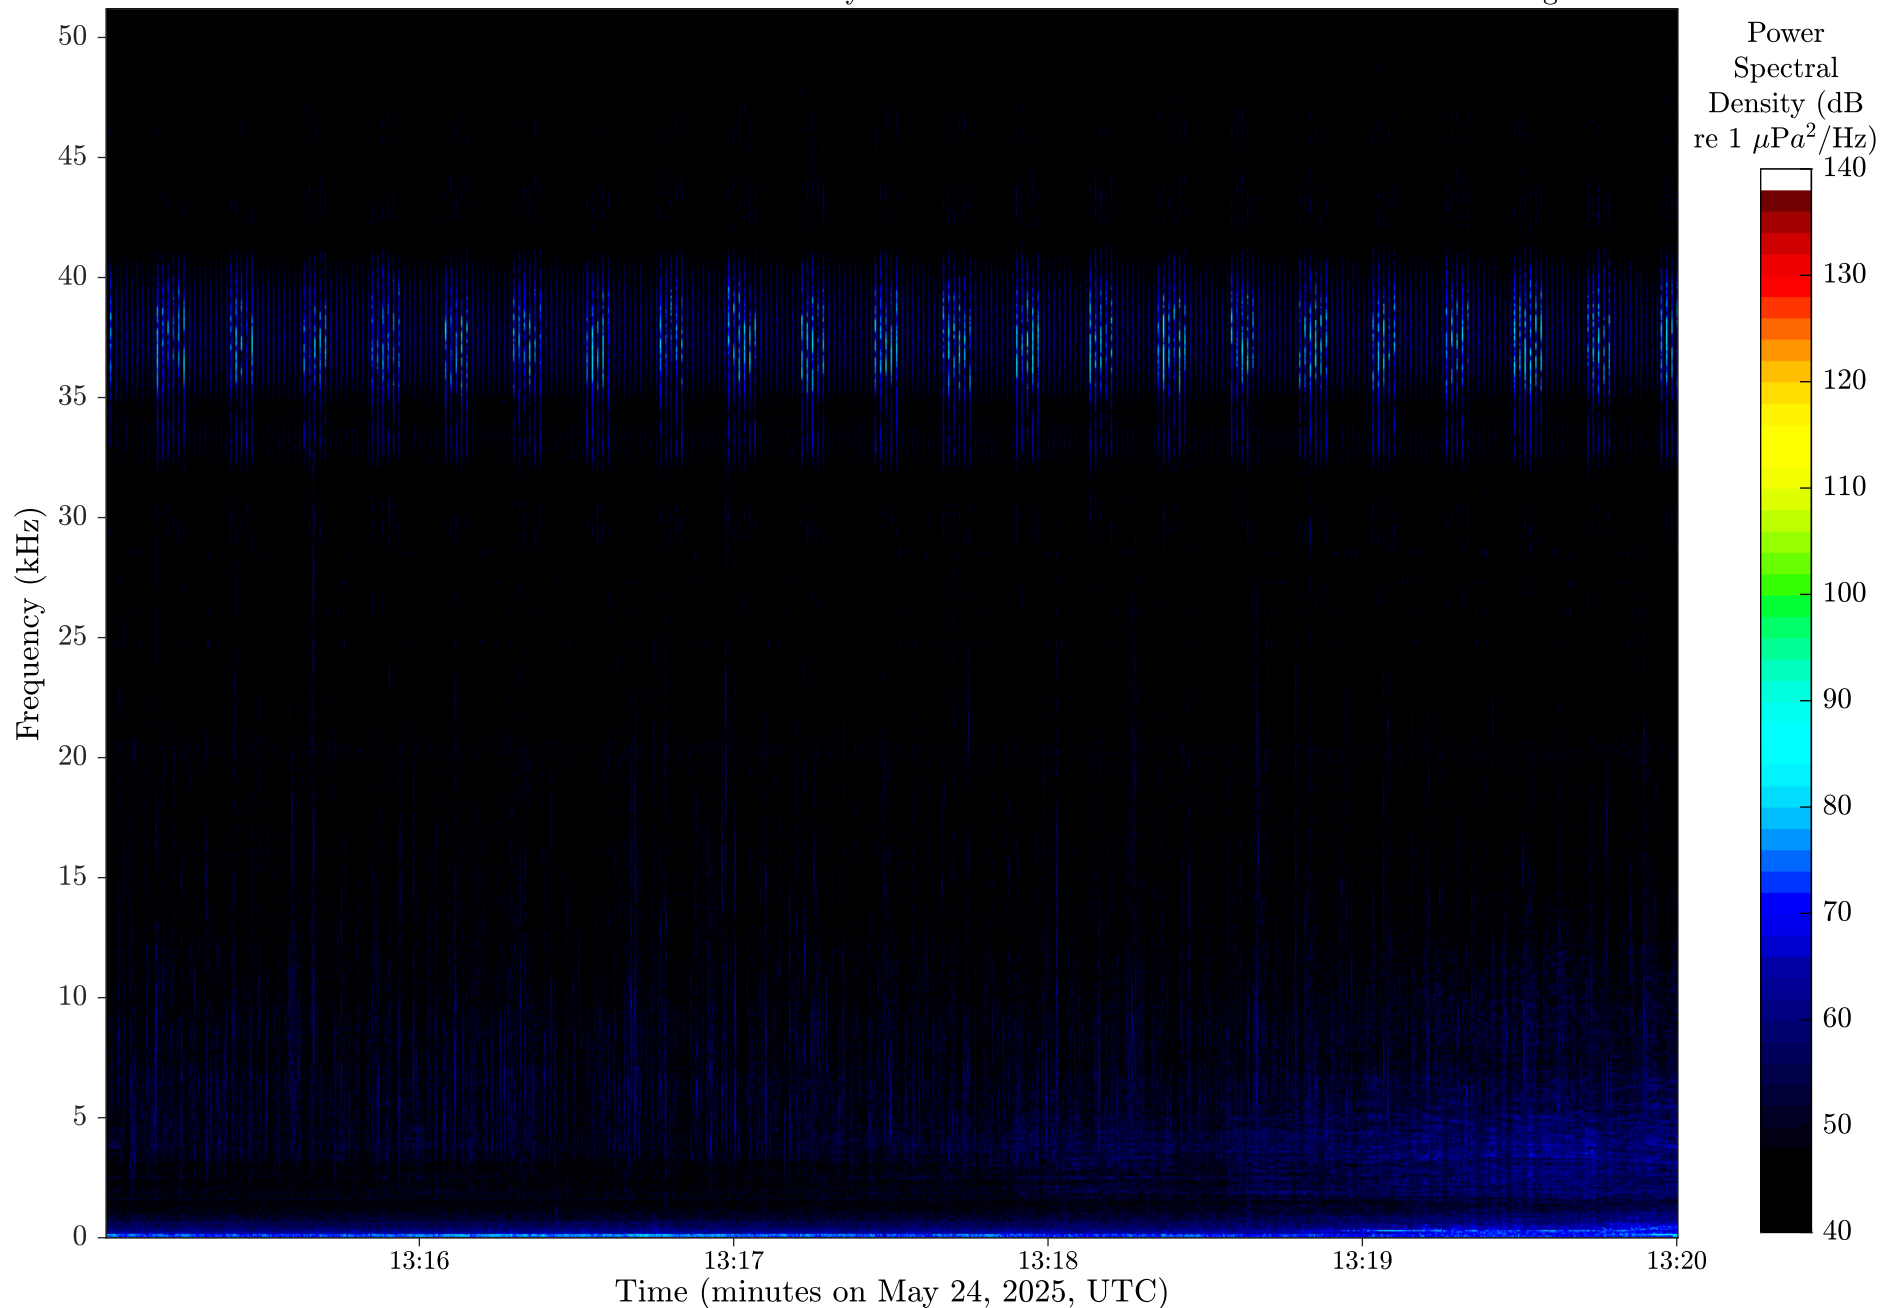

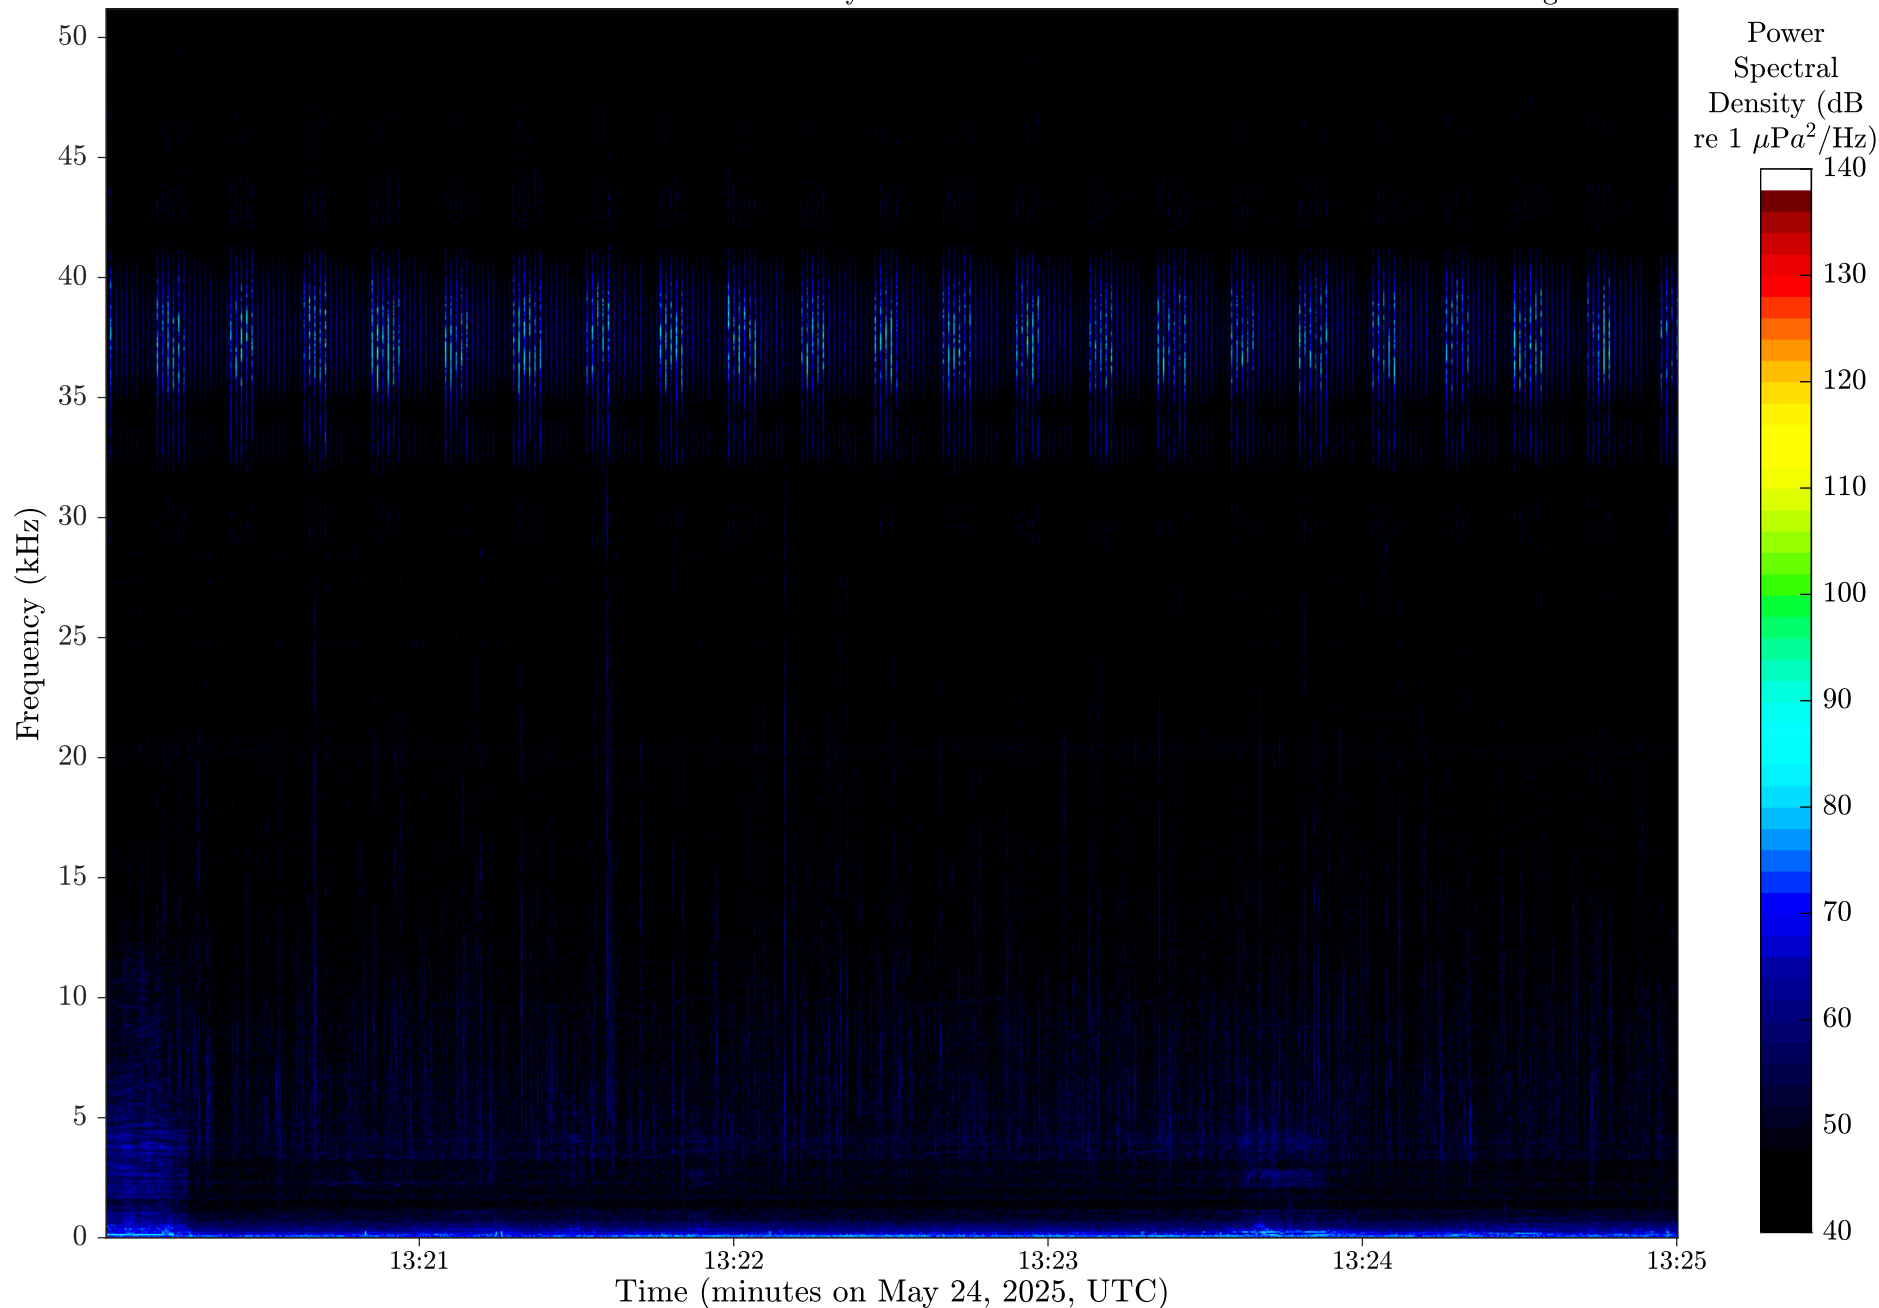


Comments: 31.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:40:54 UTC

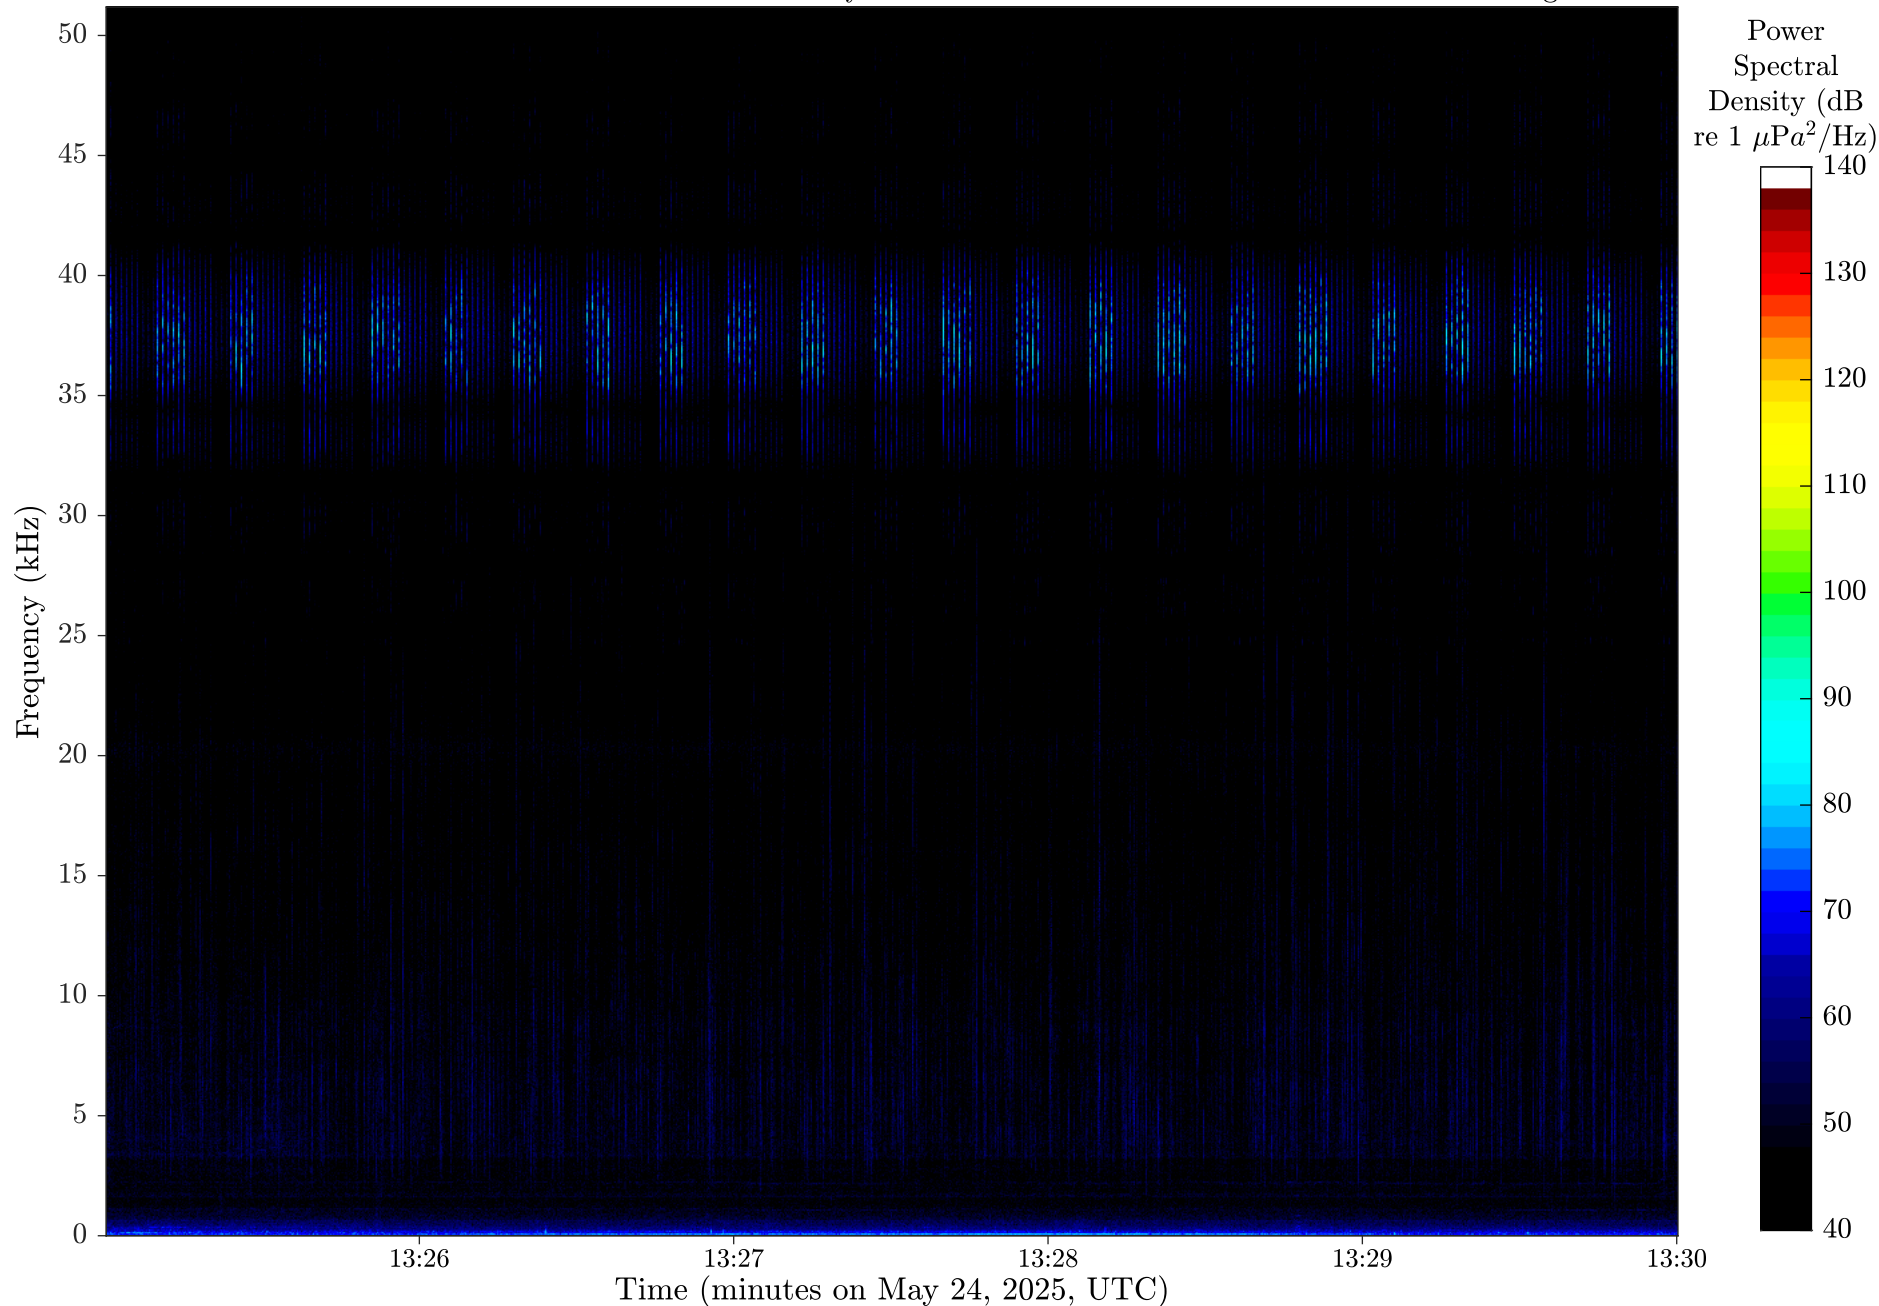


Comments: 32.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:02 UTC

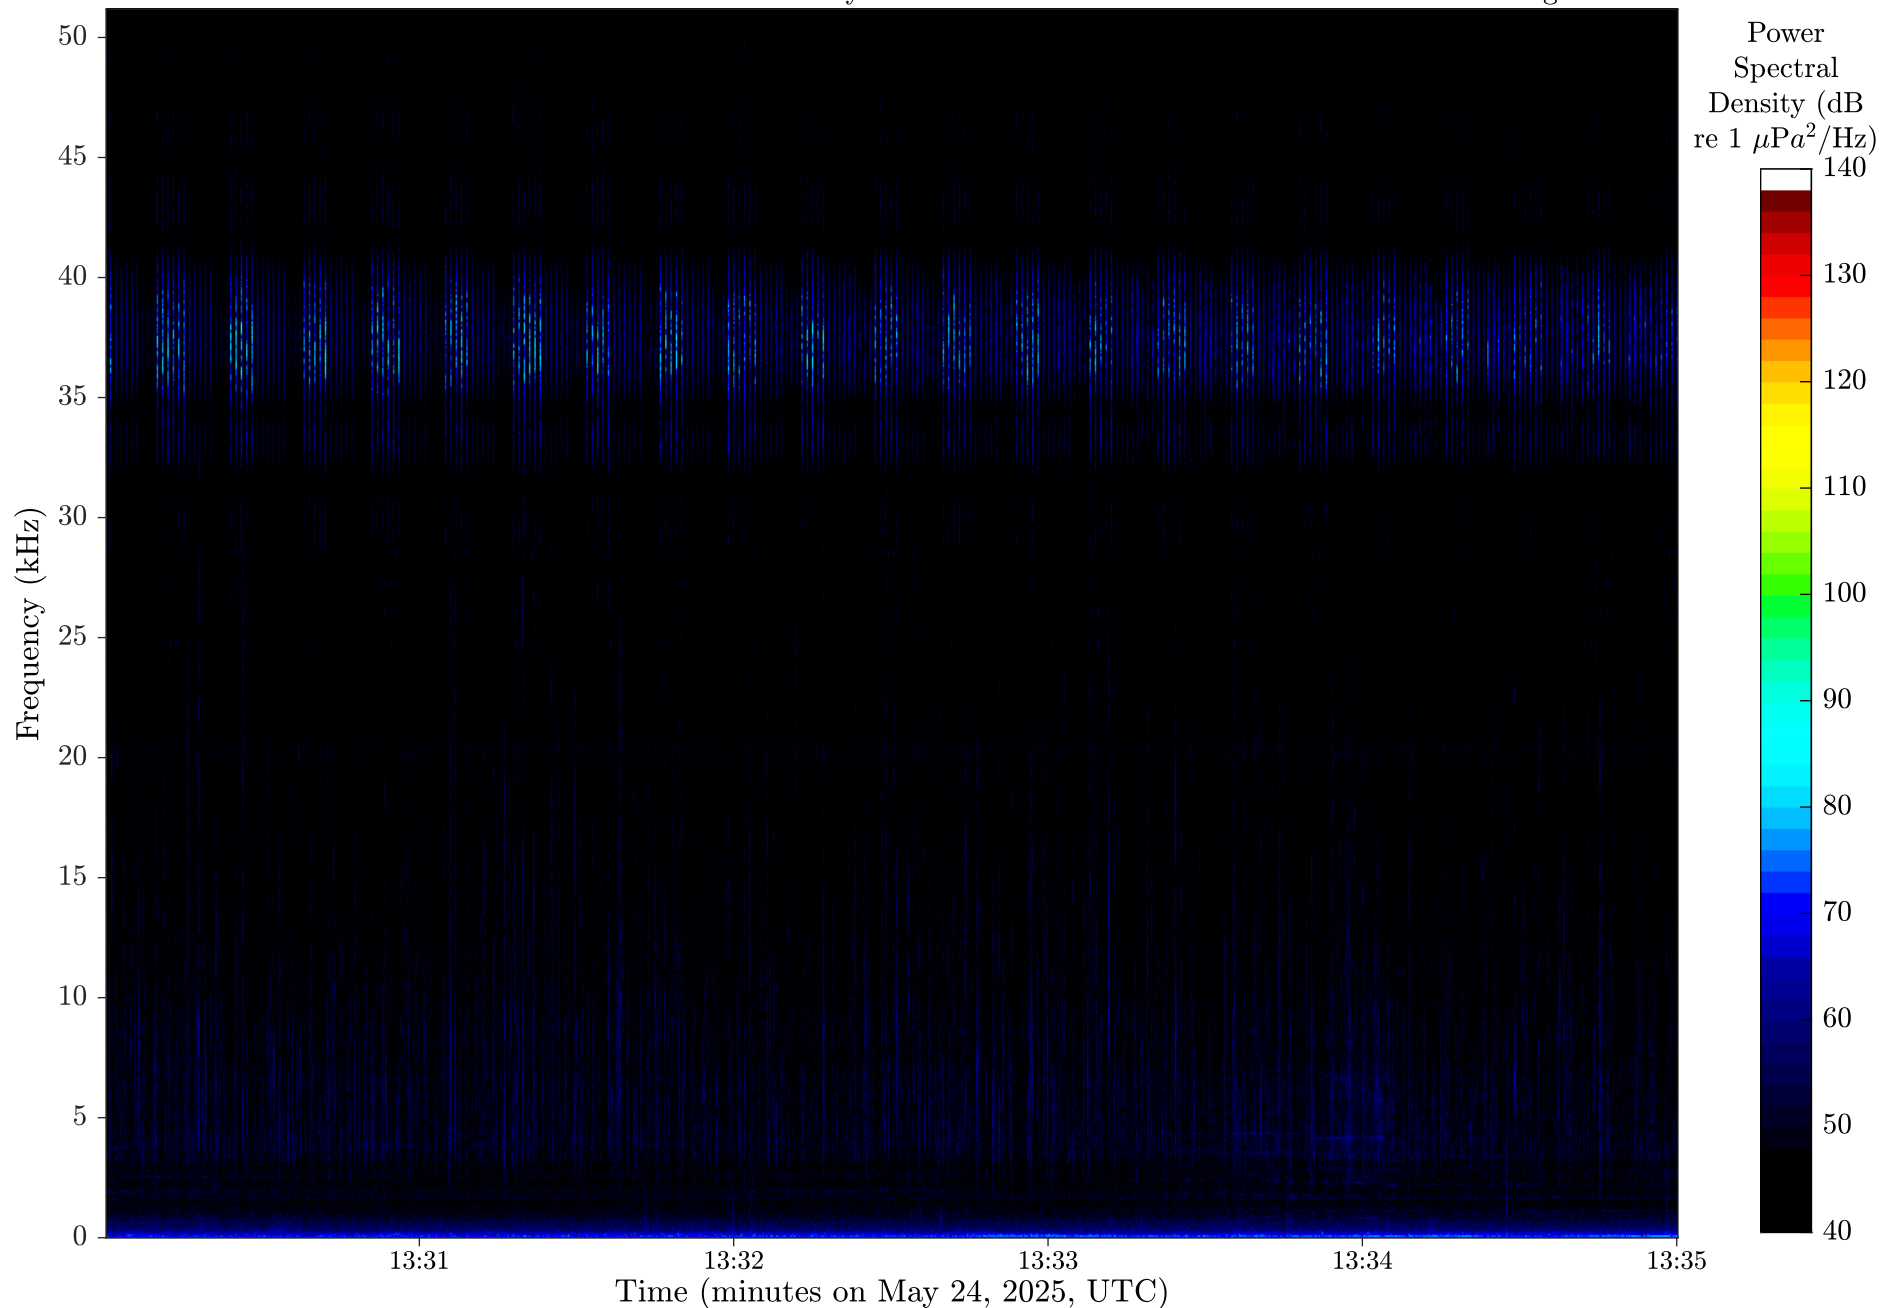


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:10 UTC

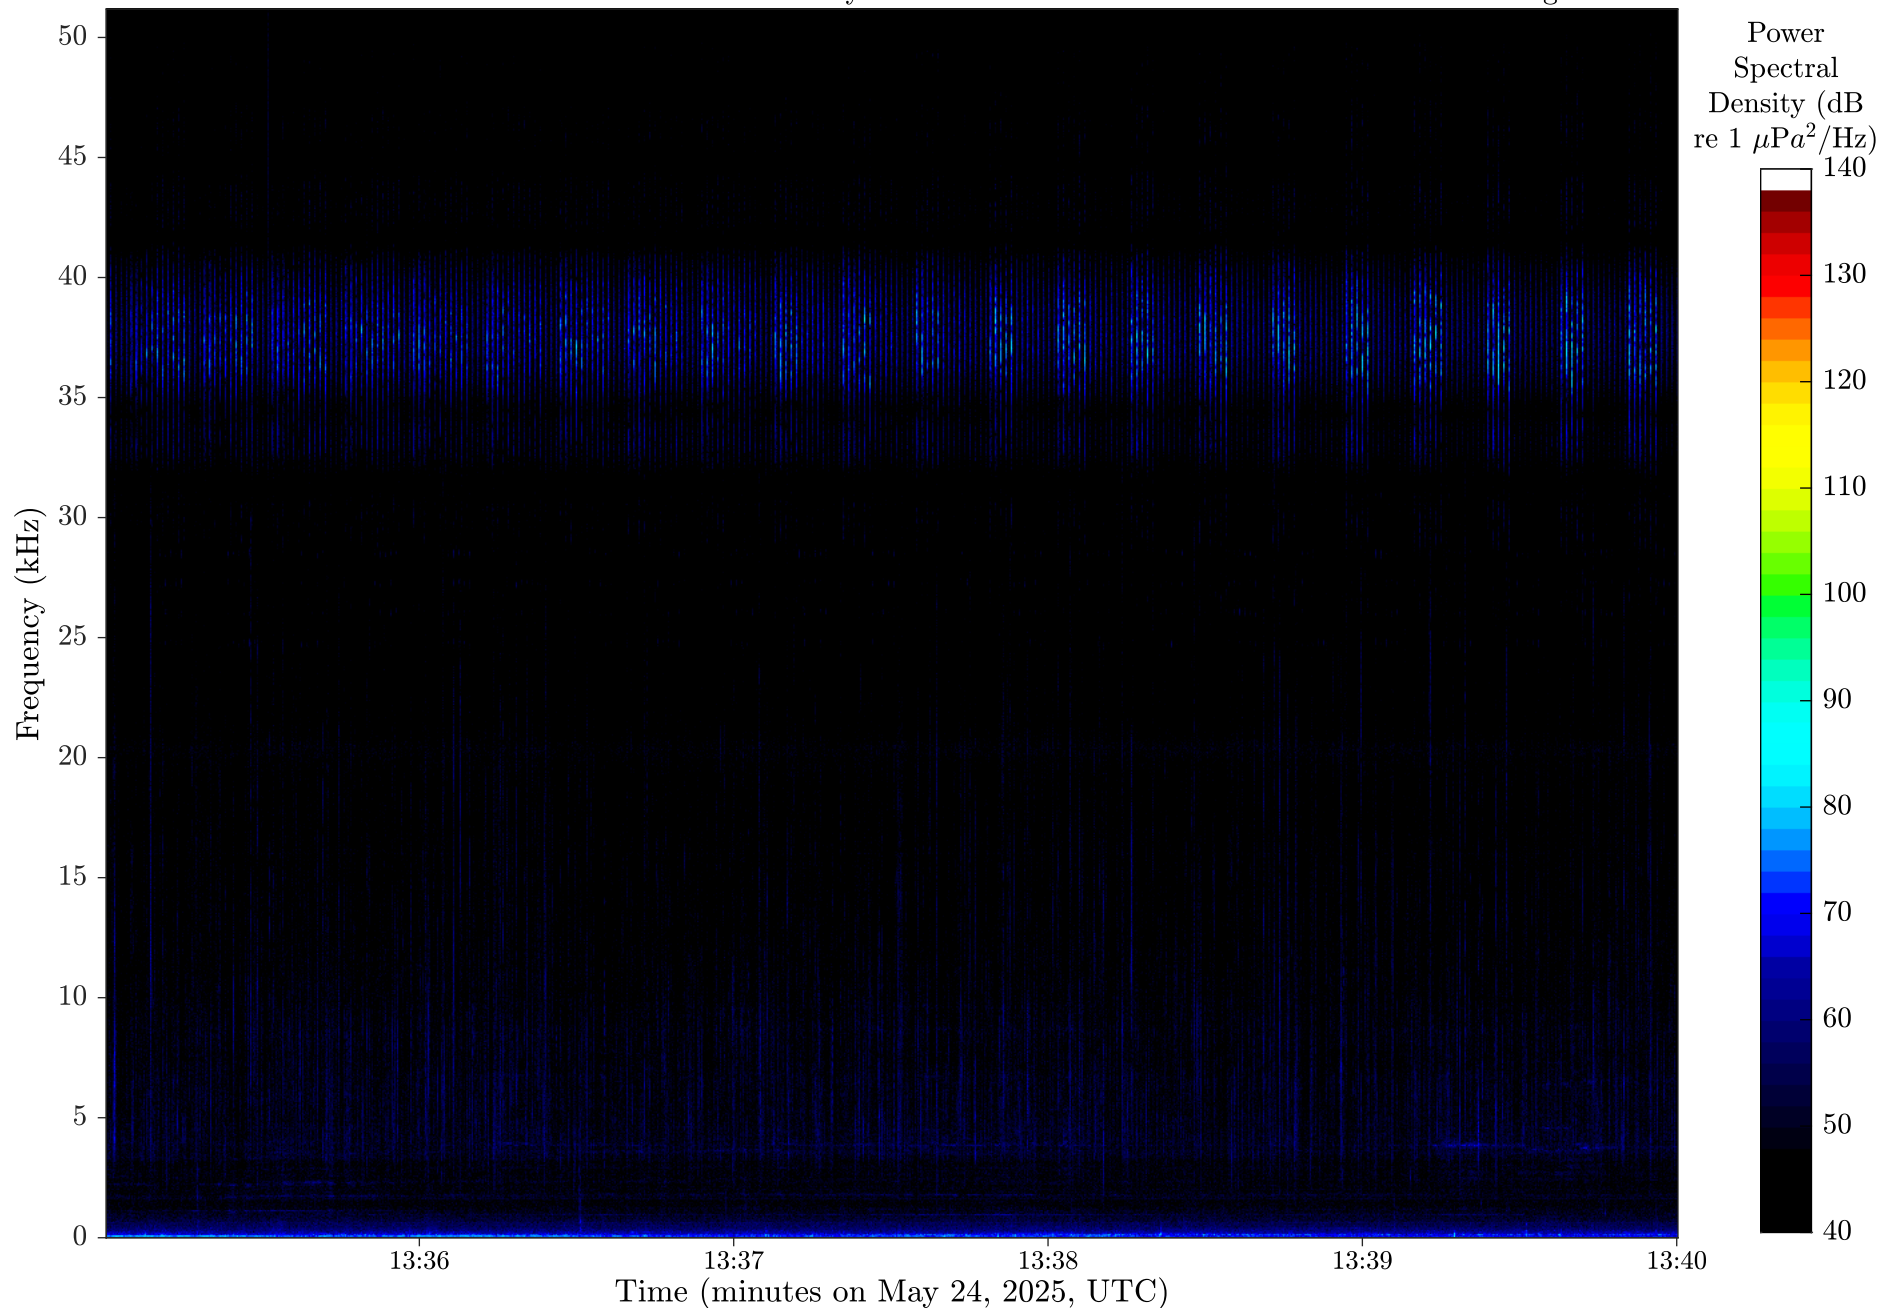


Comments: 30.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:18 UTC

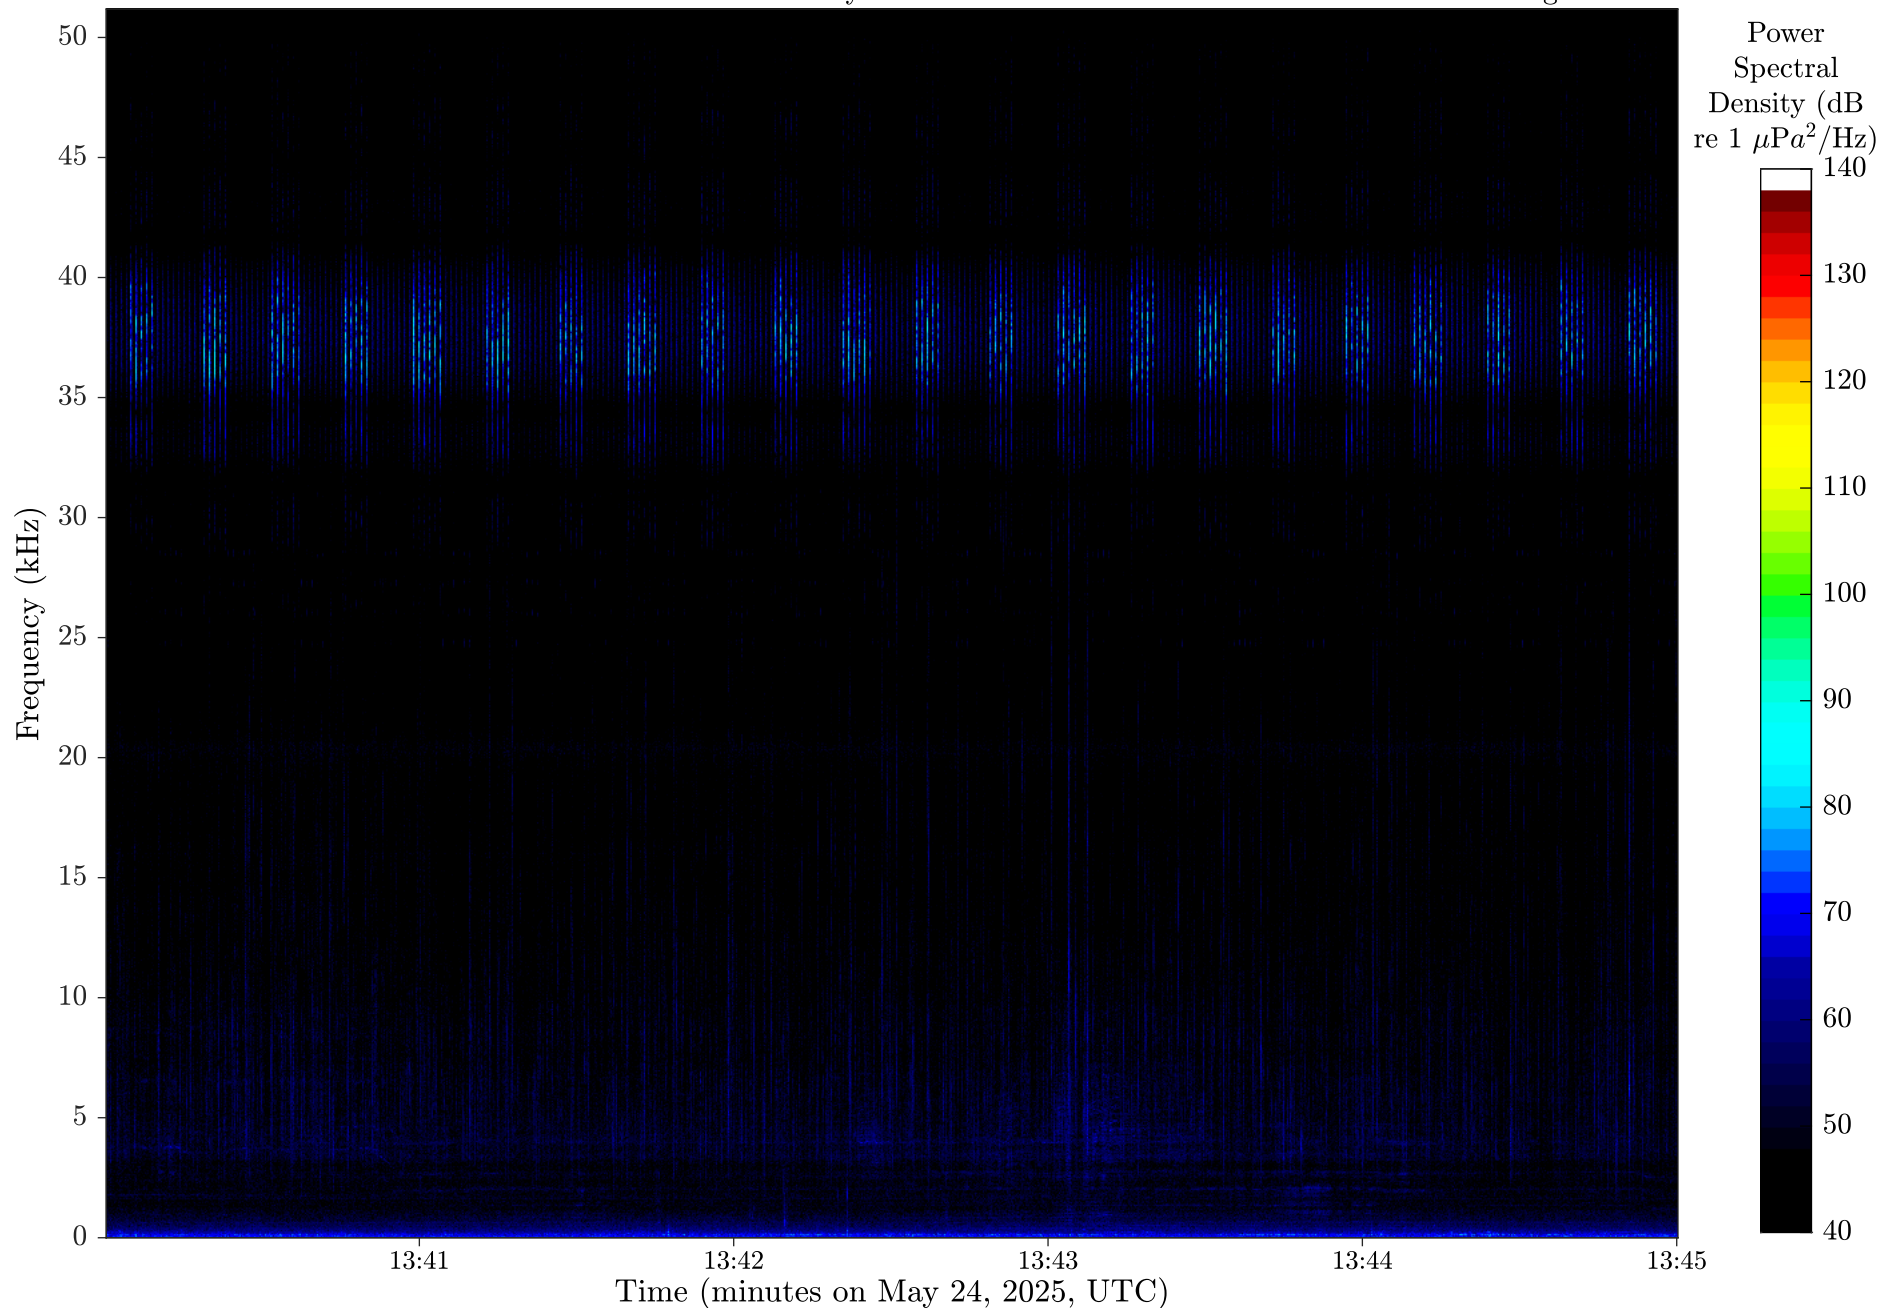


Comments: 31.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:26 UTC

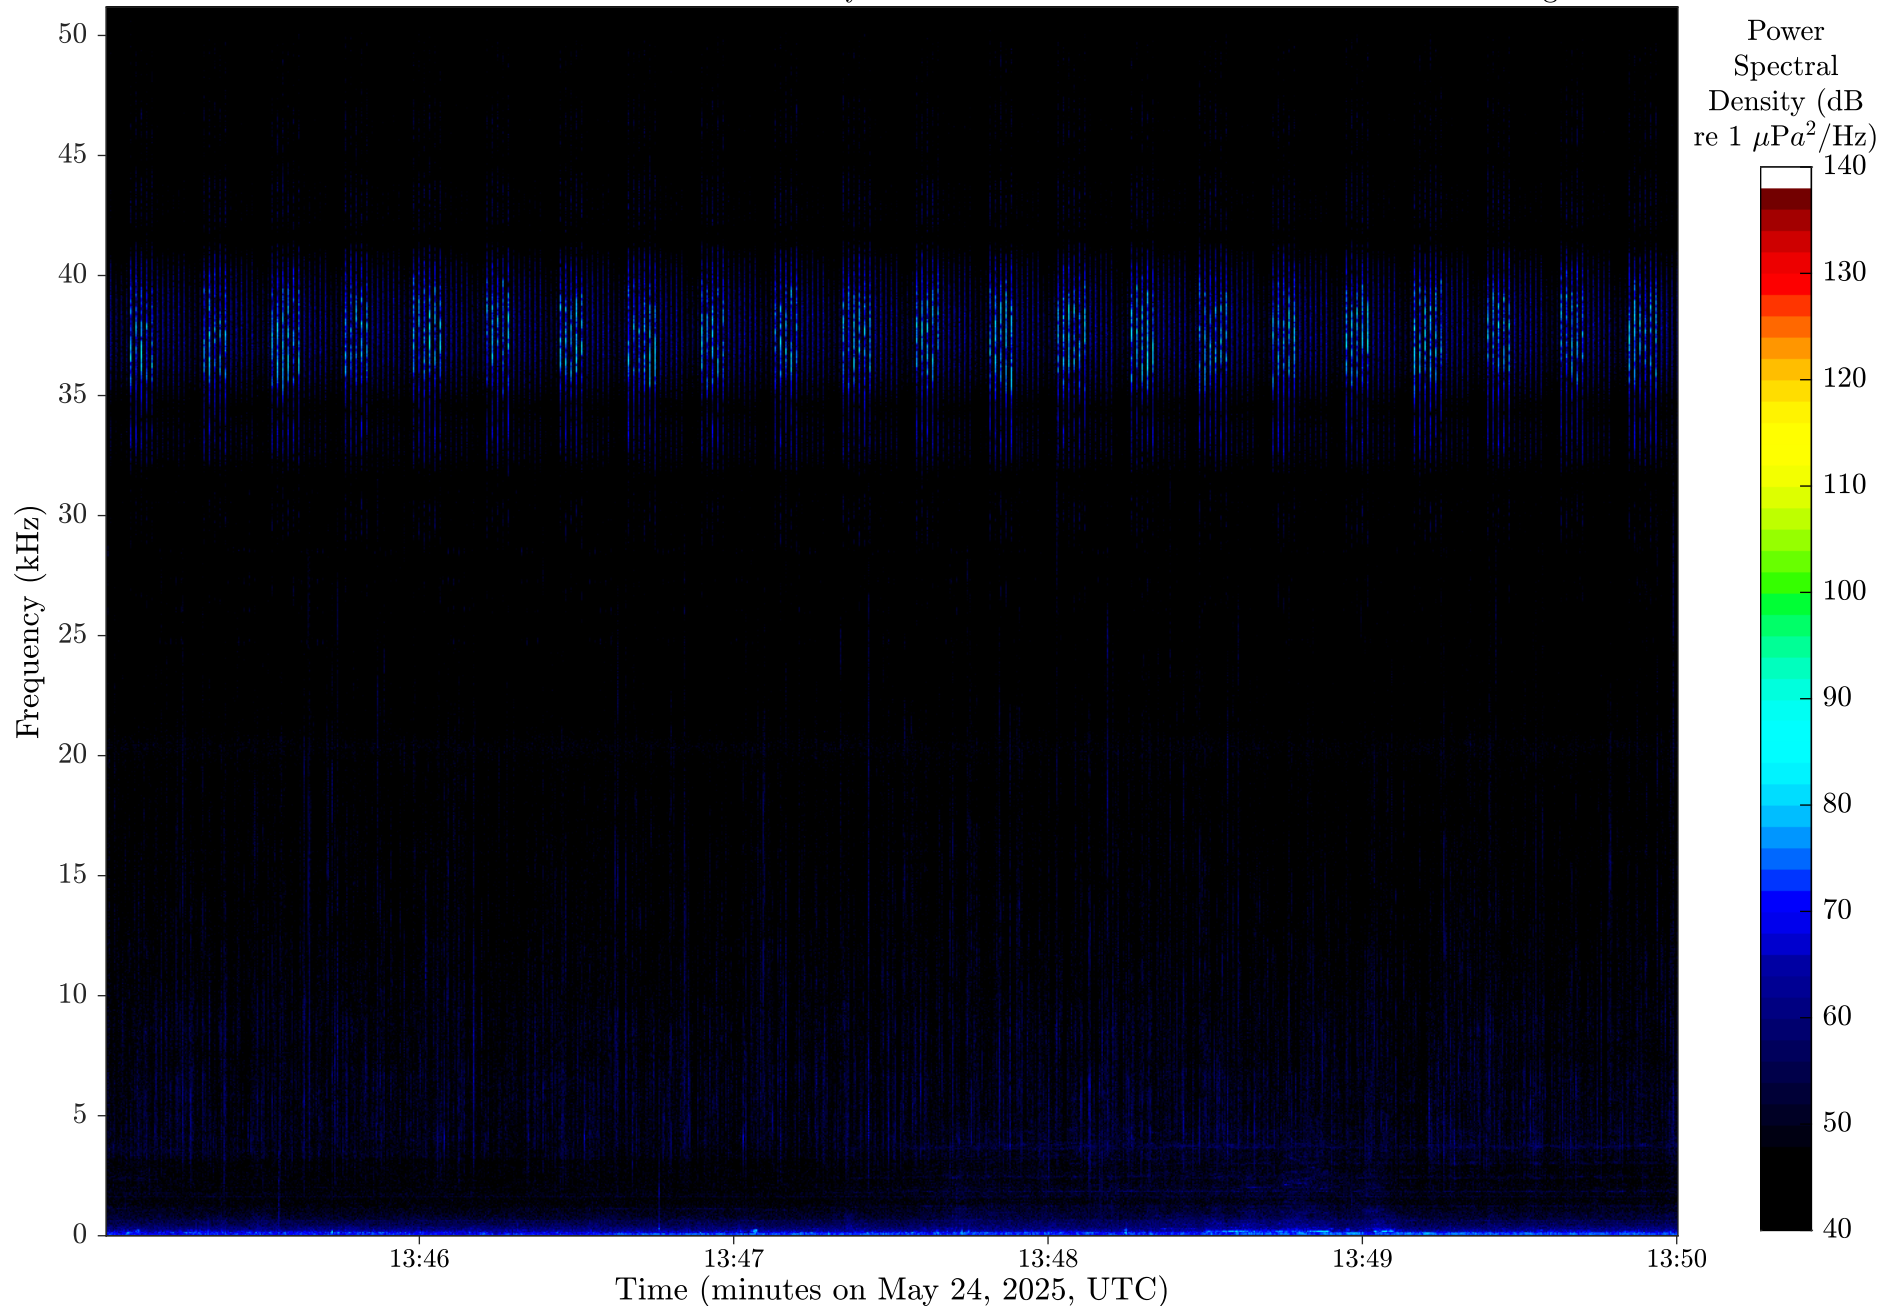


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:34 UTC

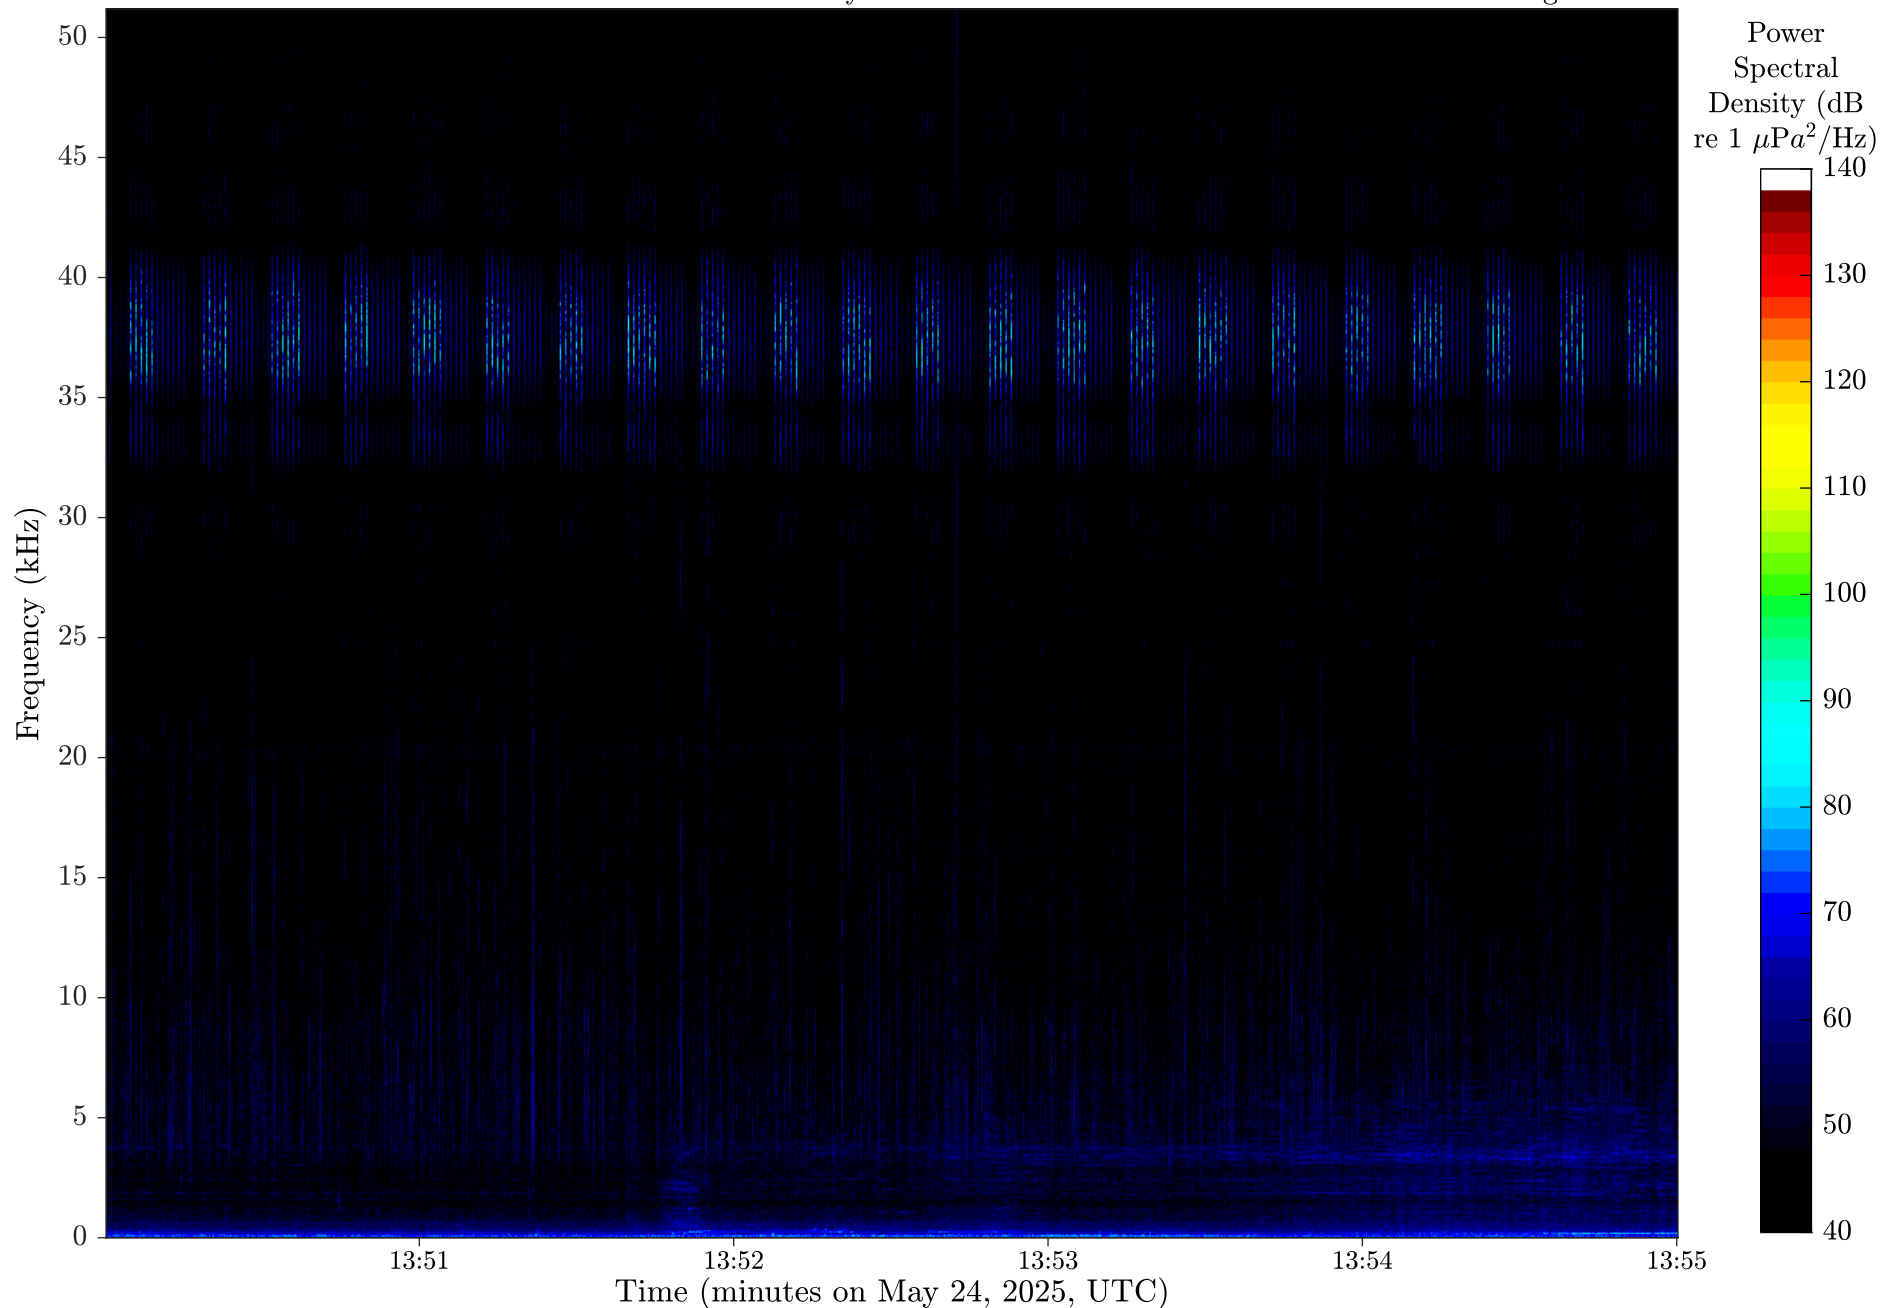


Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:43 UTC

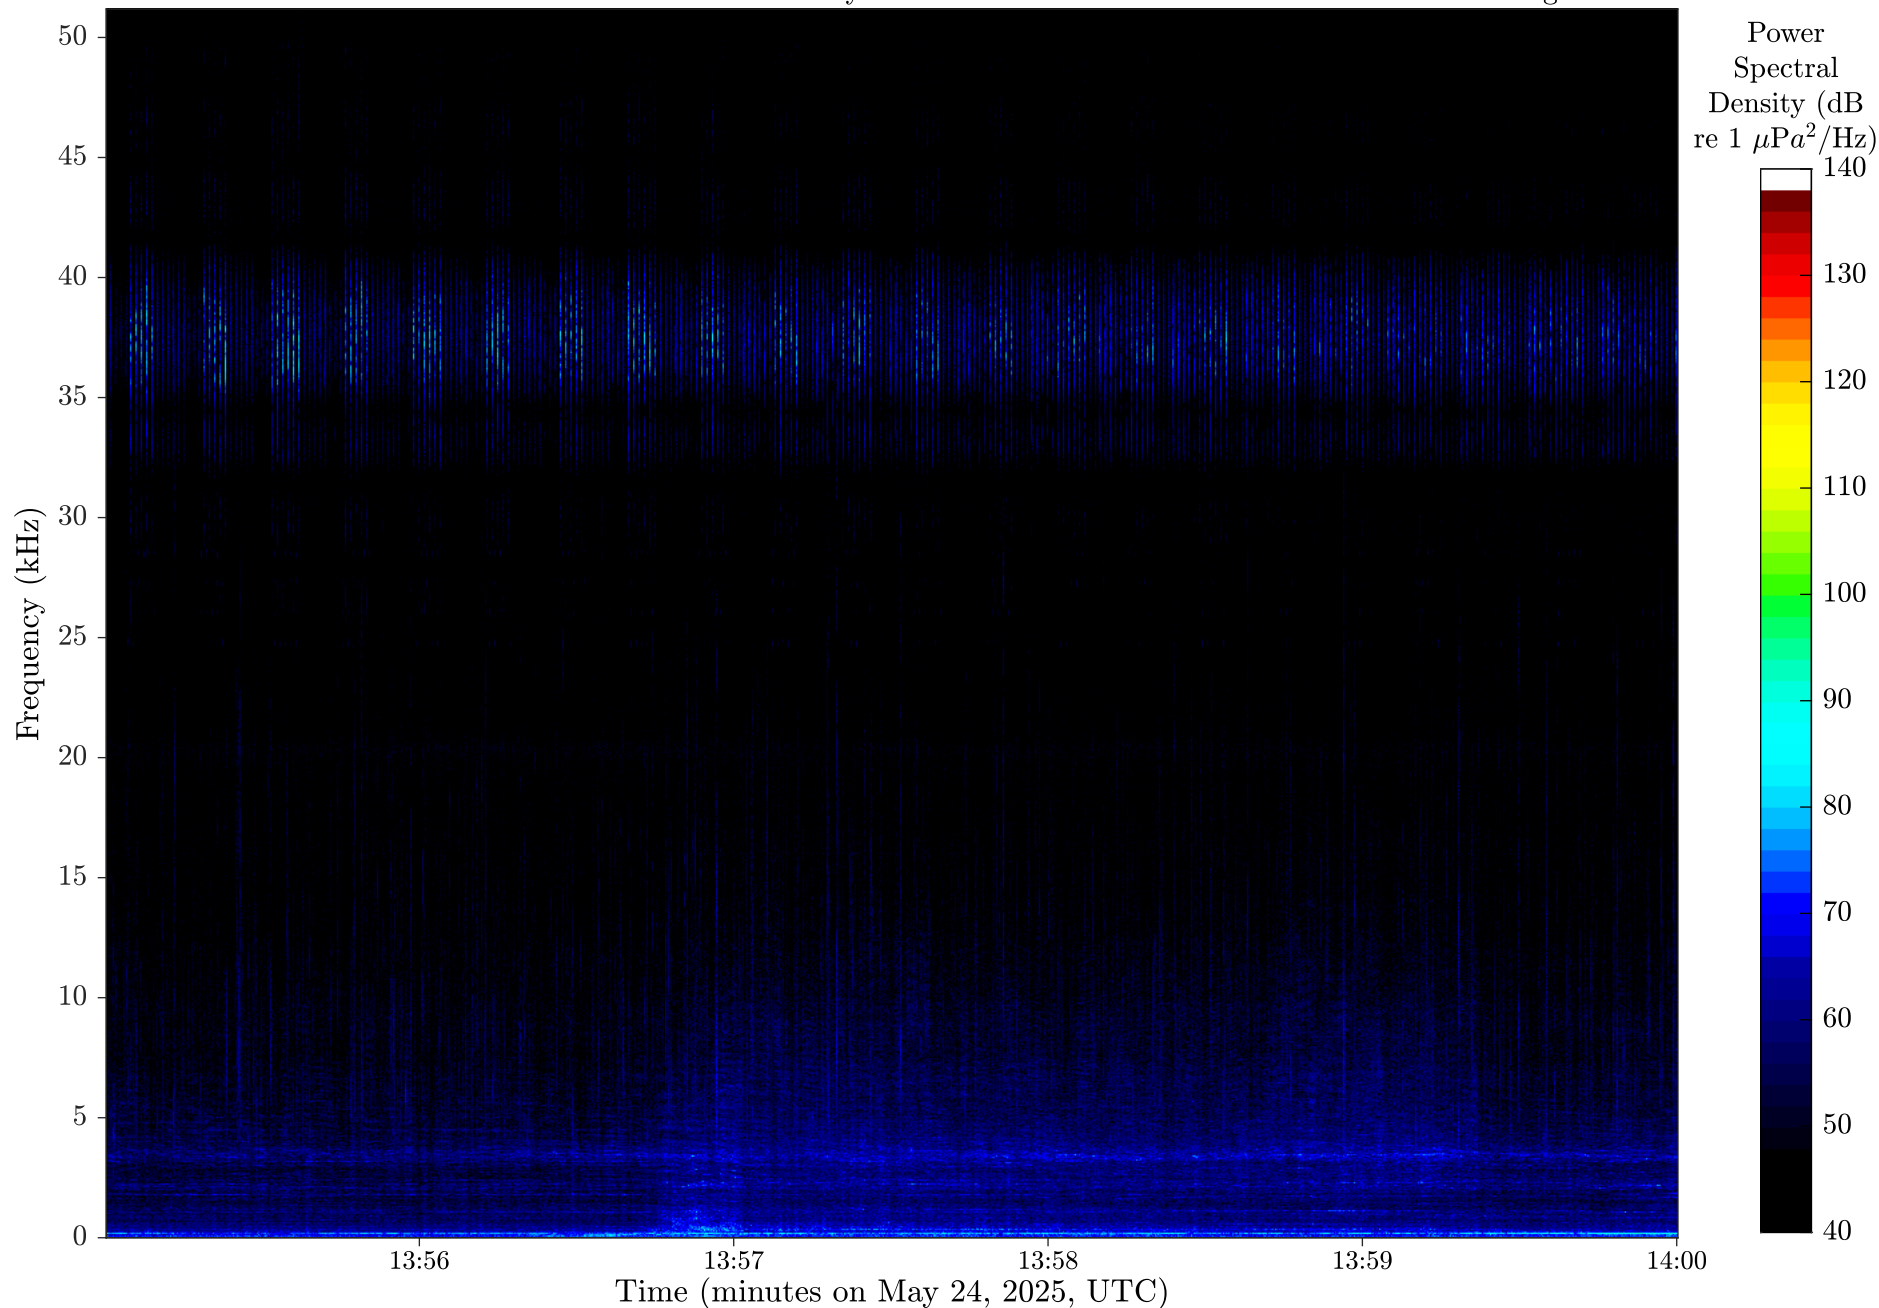


Comments: 29.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:50 UTC

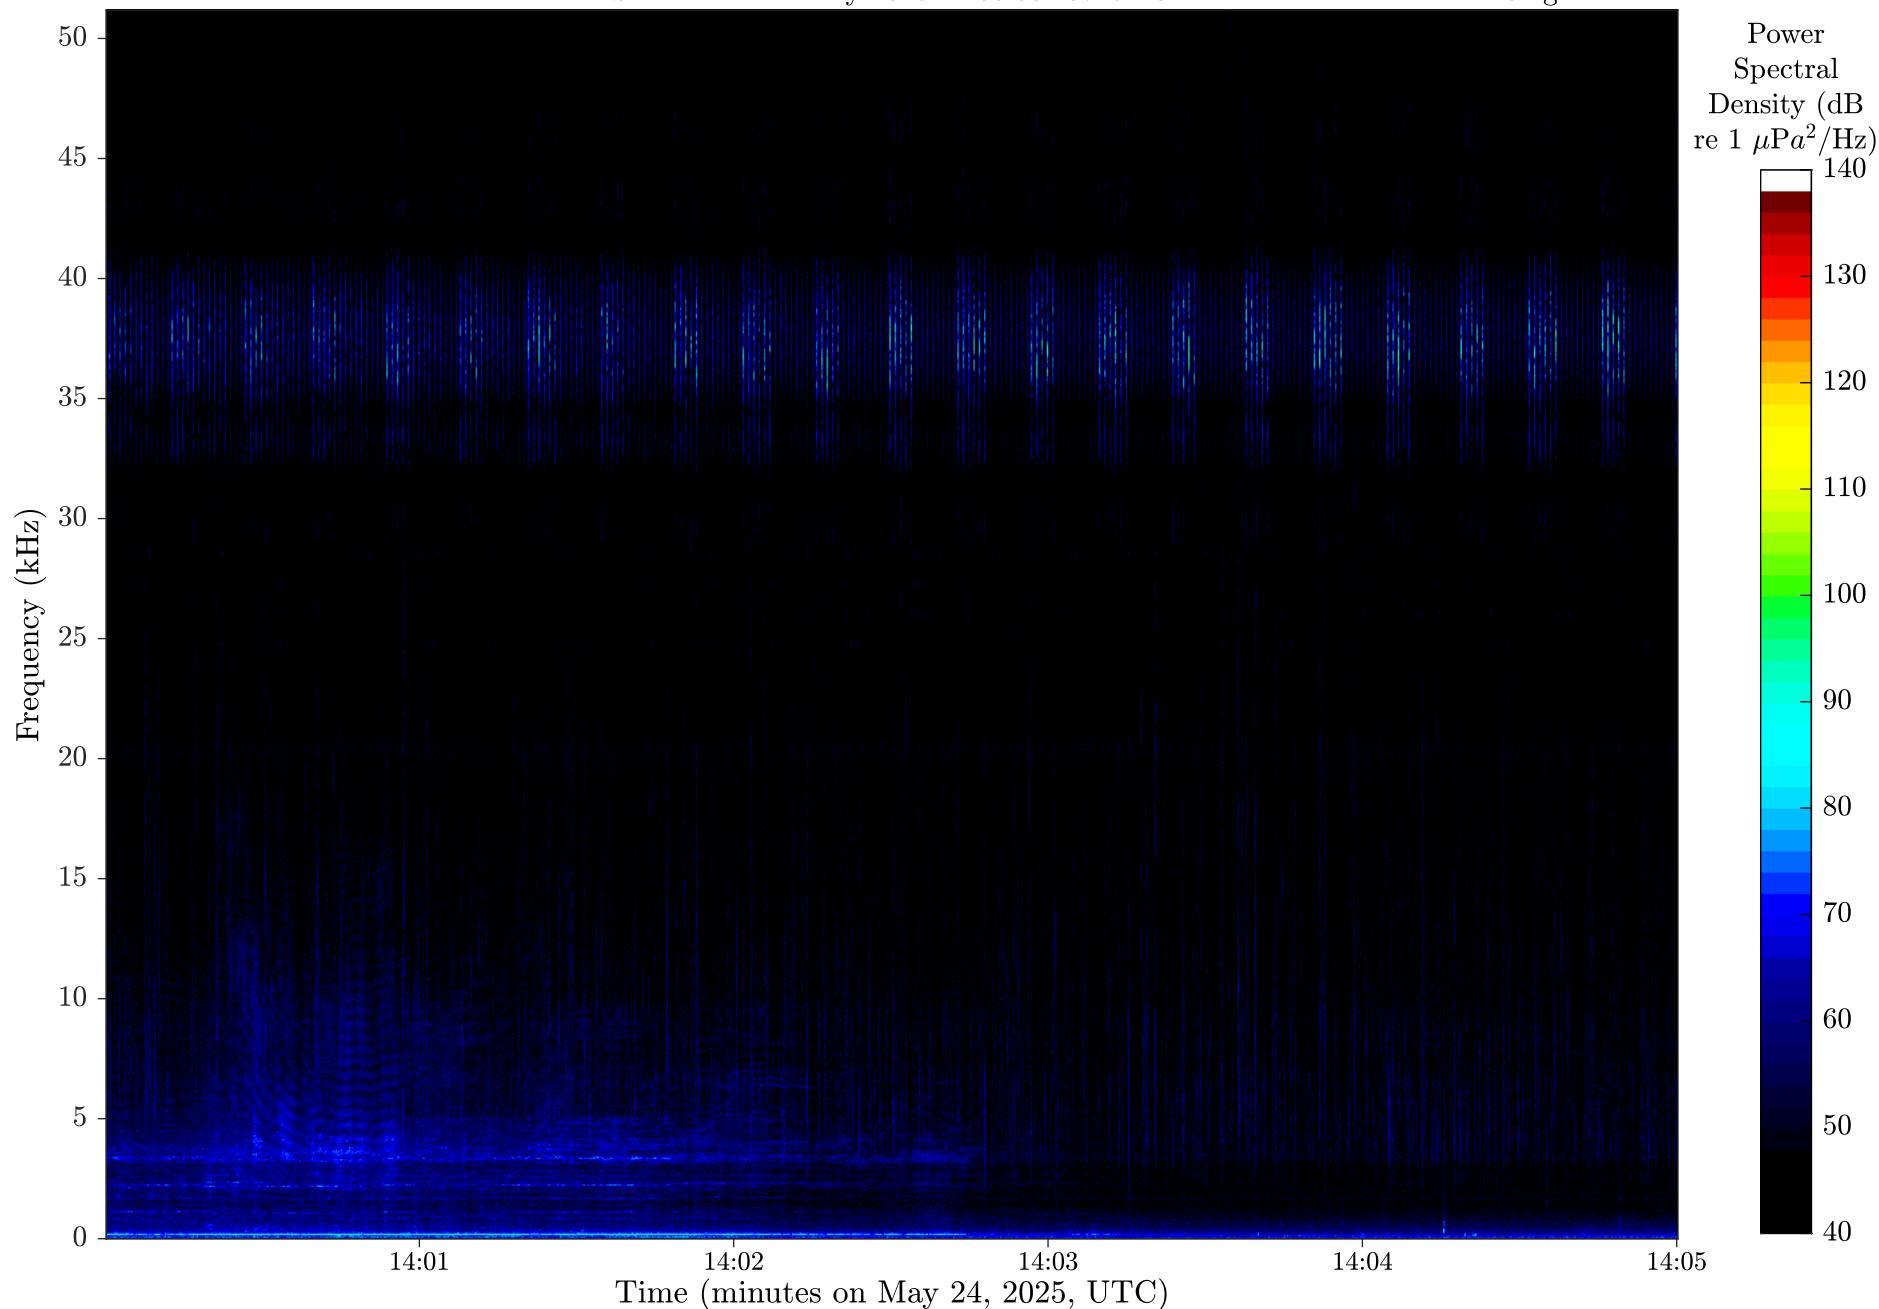


Comments: 31.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:41:58 UTC

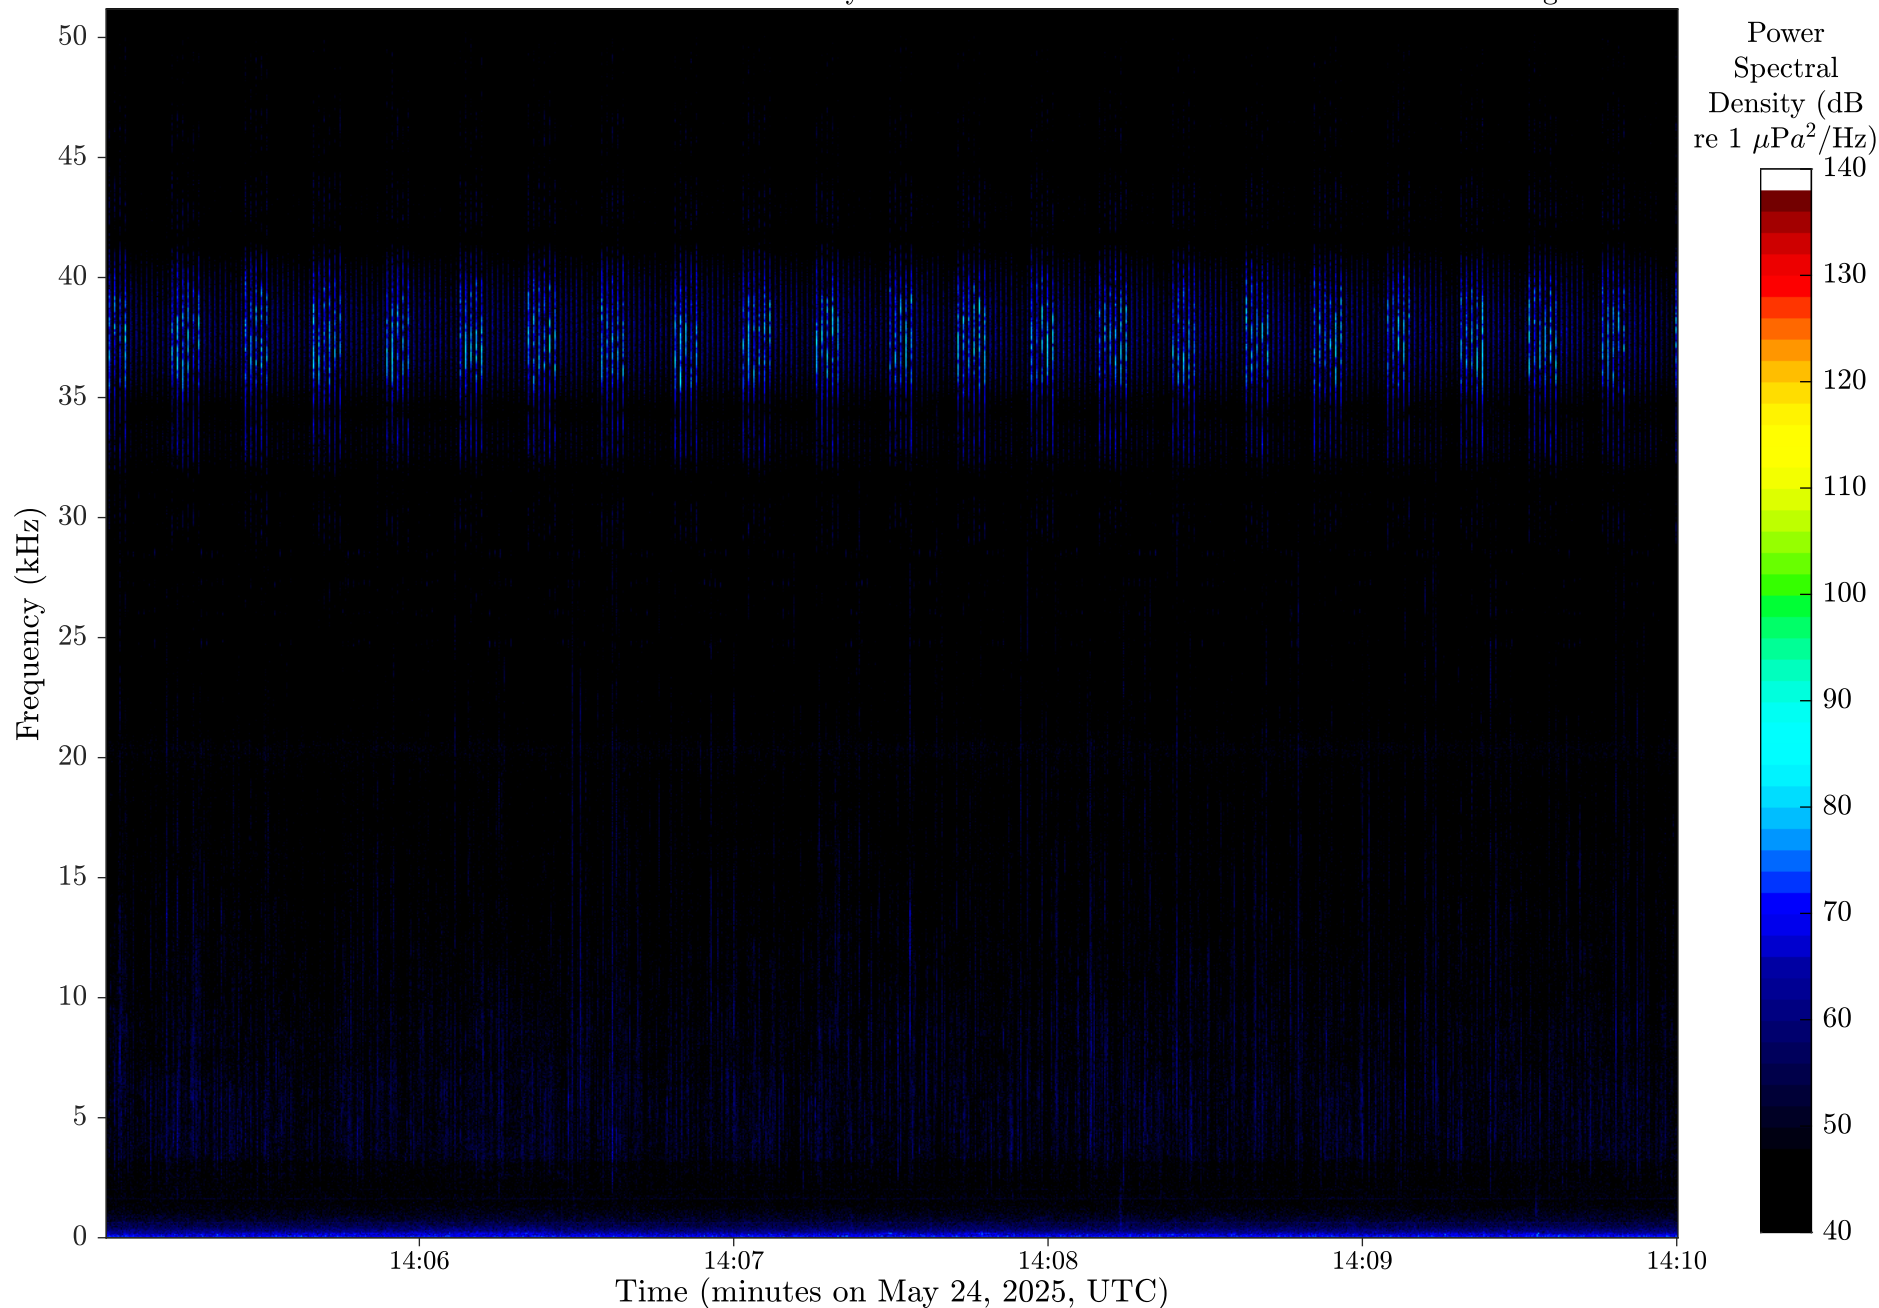


Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:06 UTC

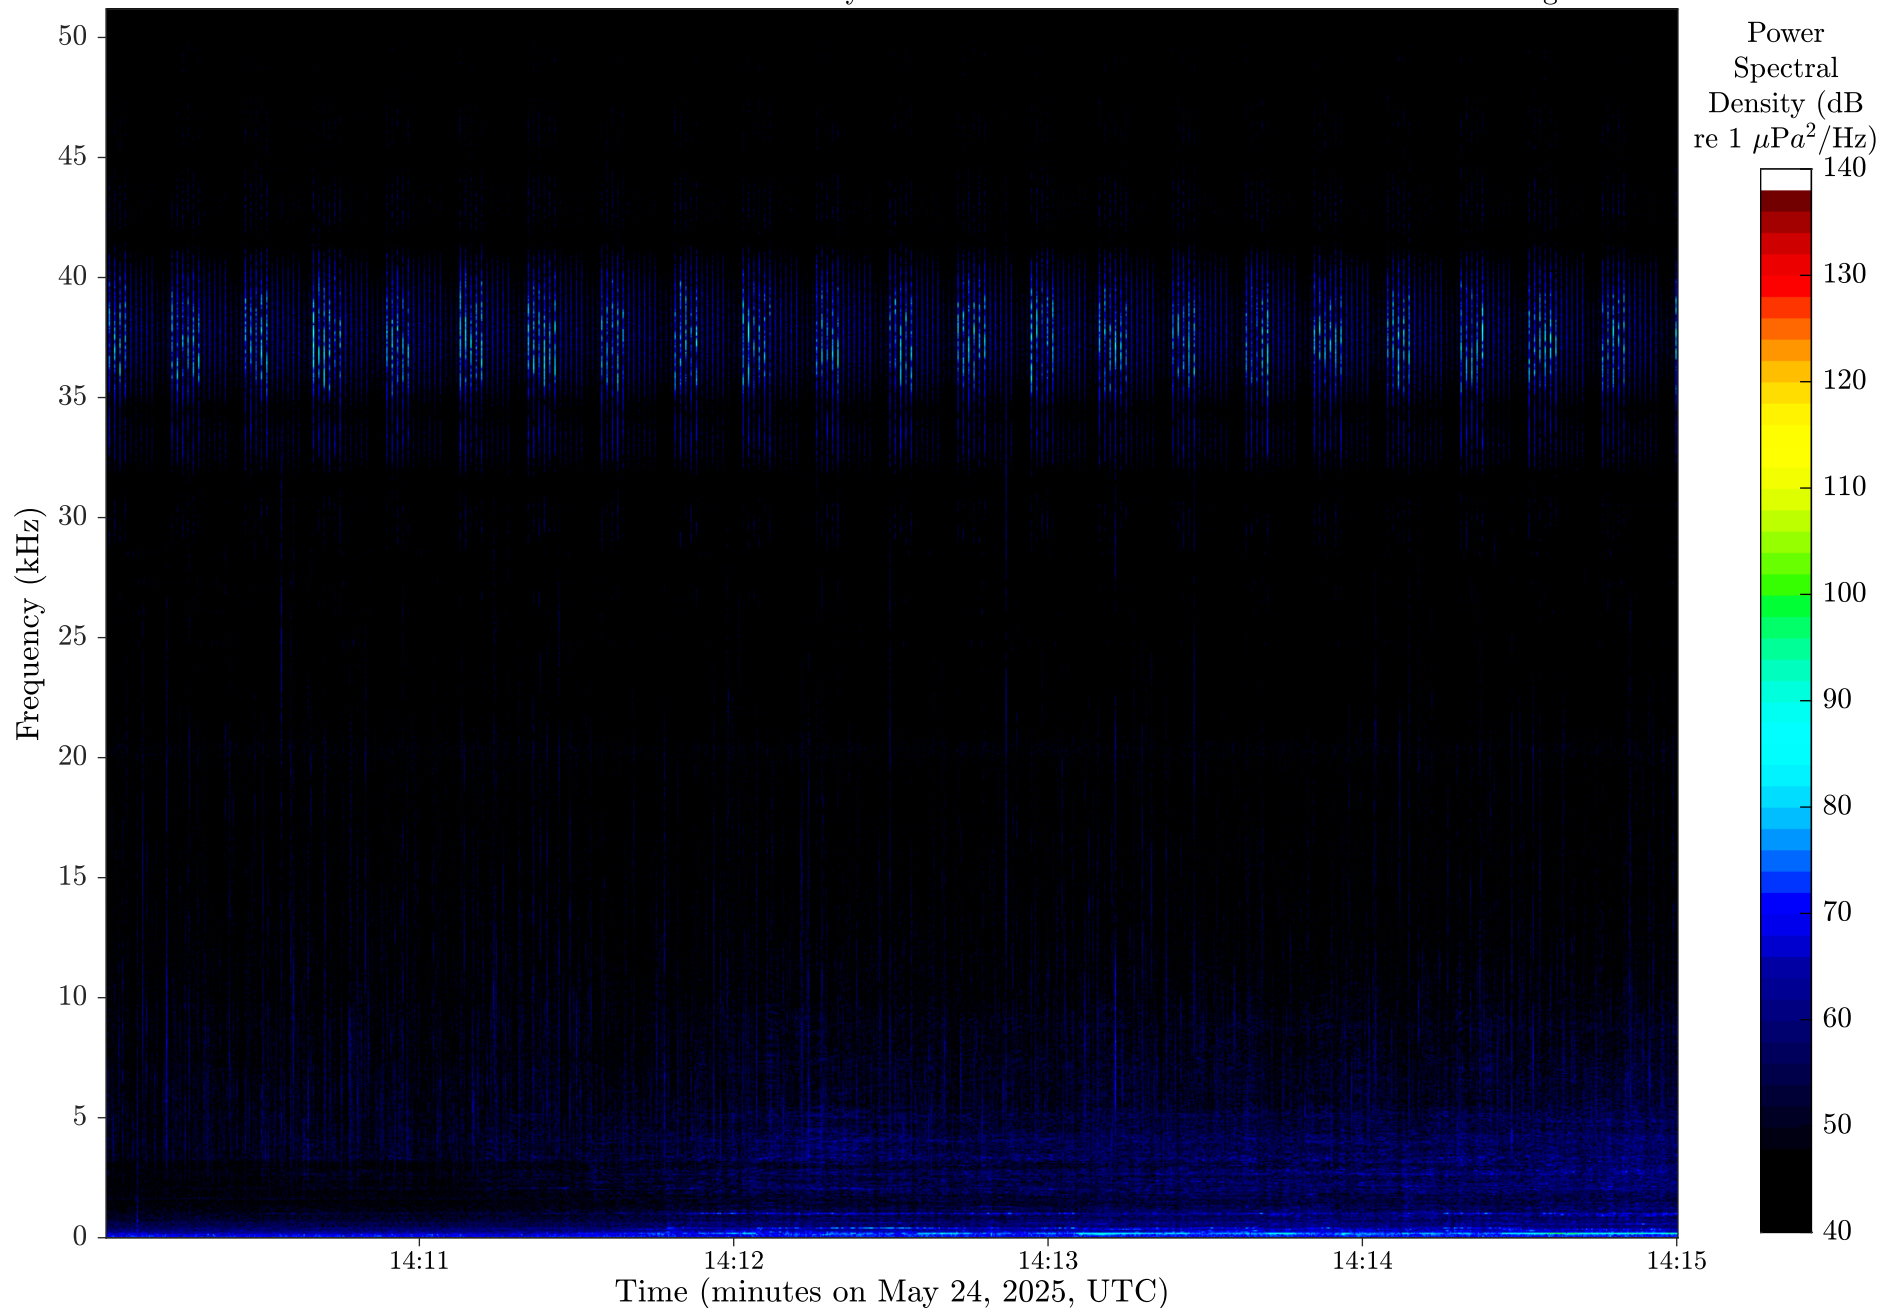


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:15 UTC

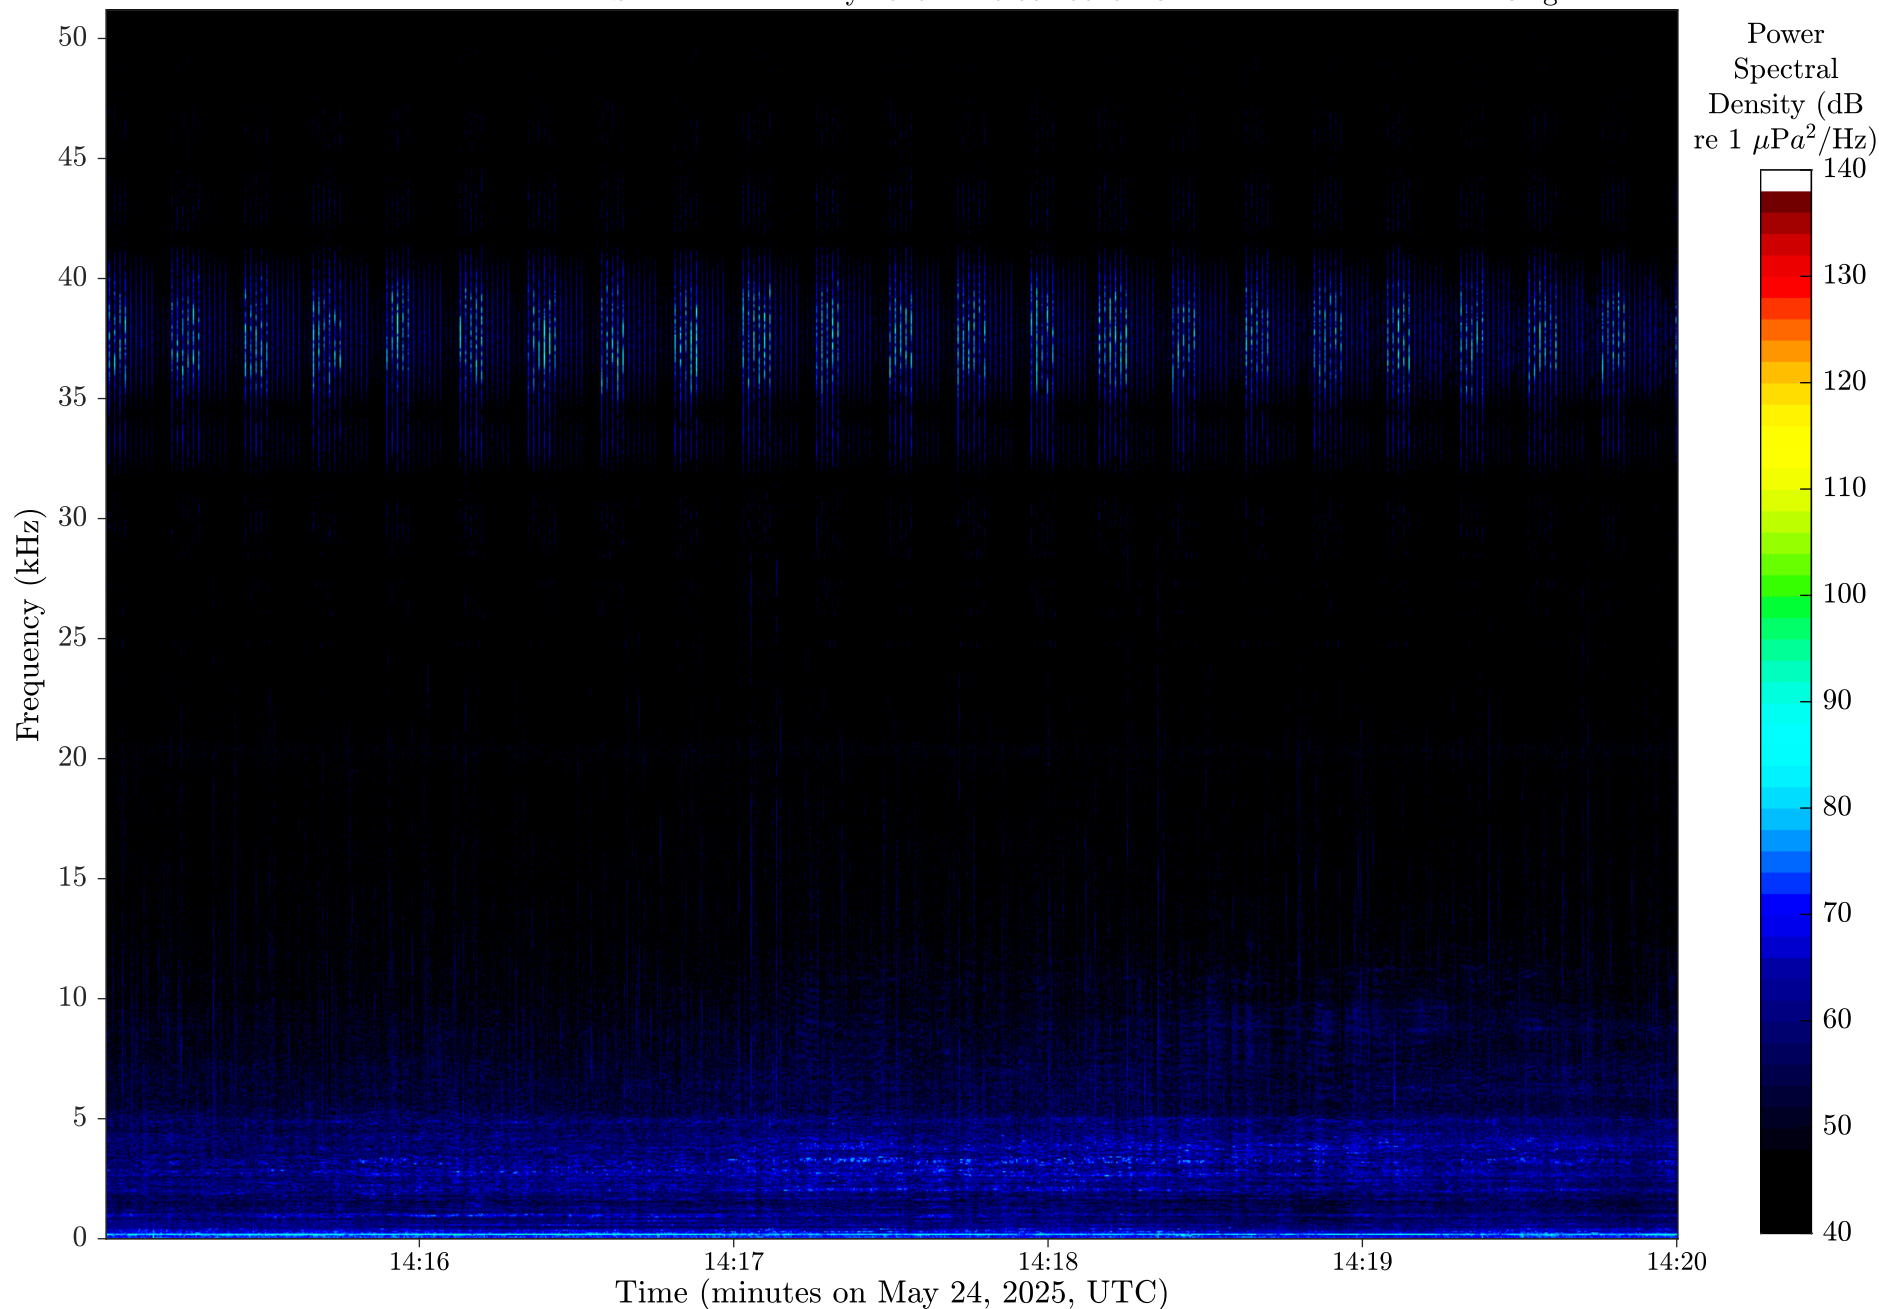


Comments: 31.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:23 UTC

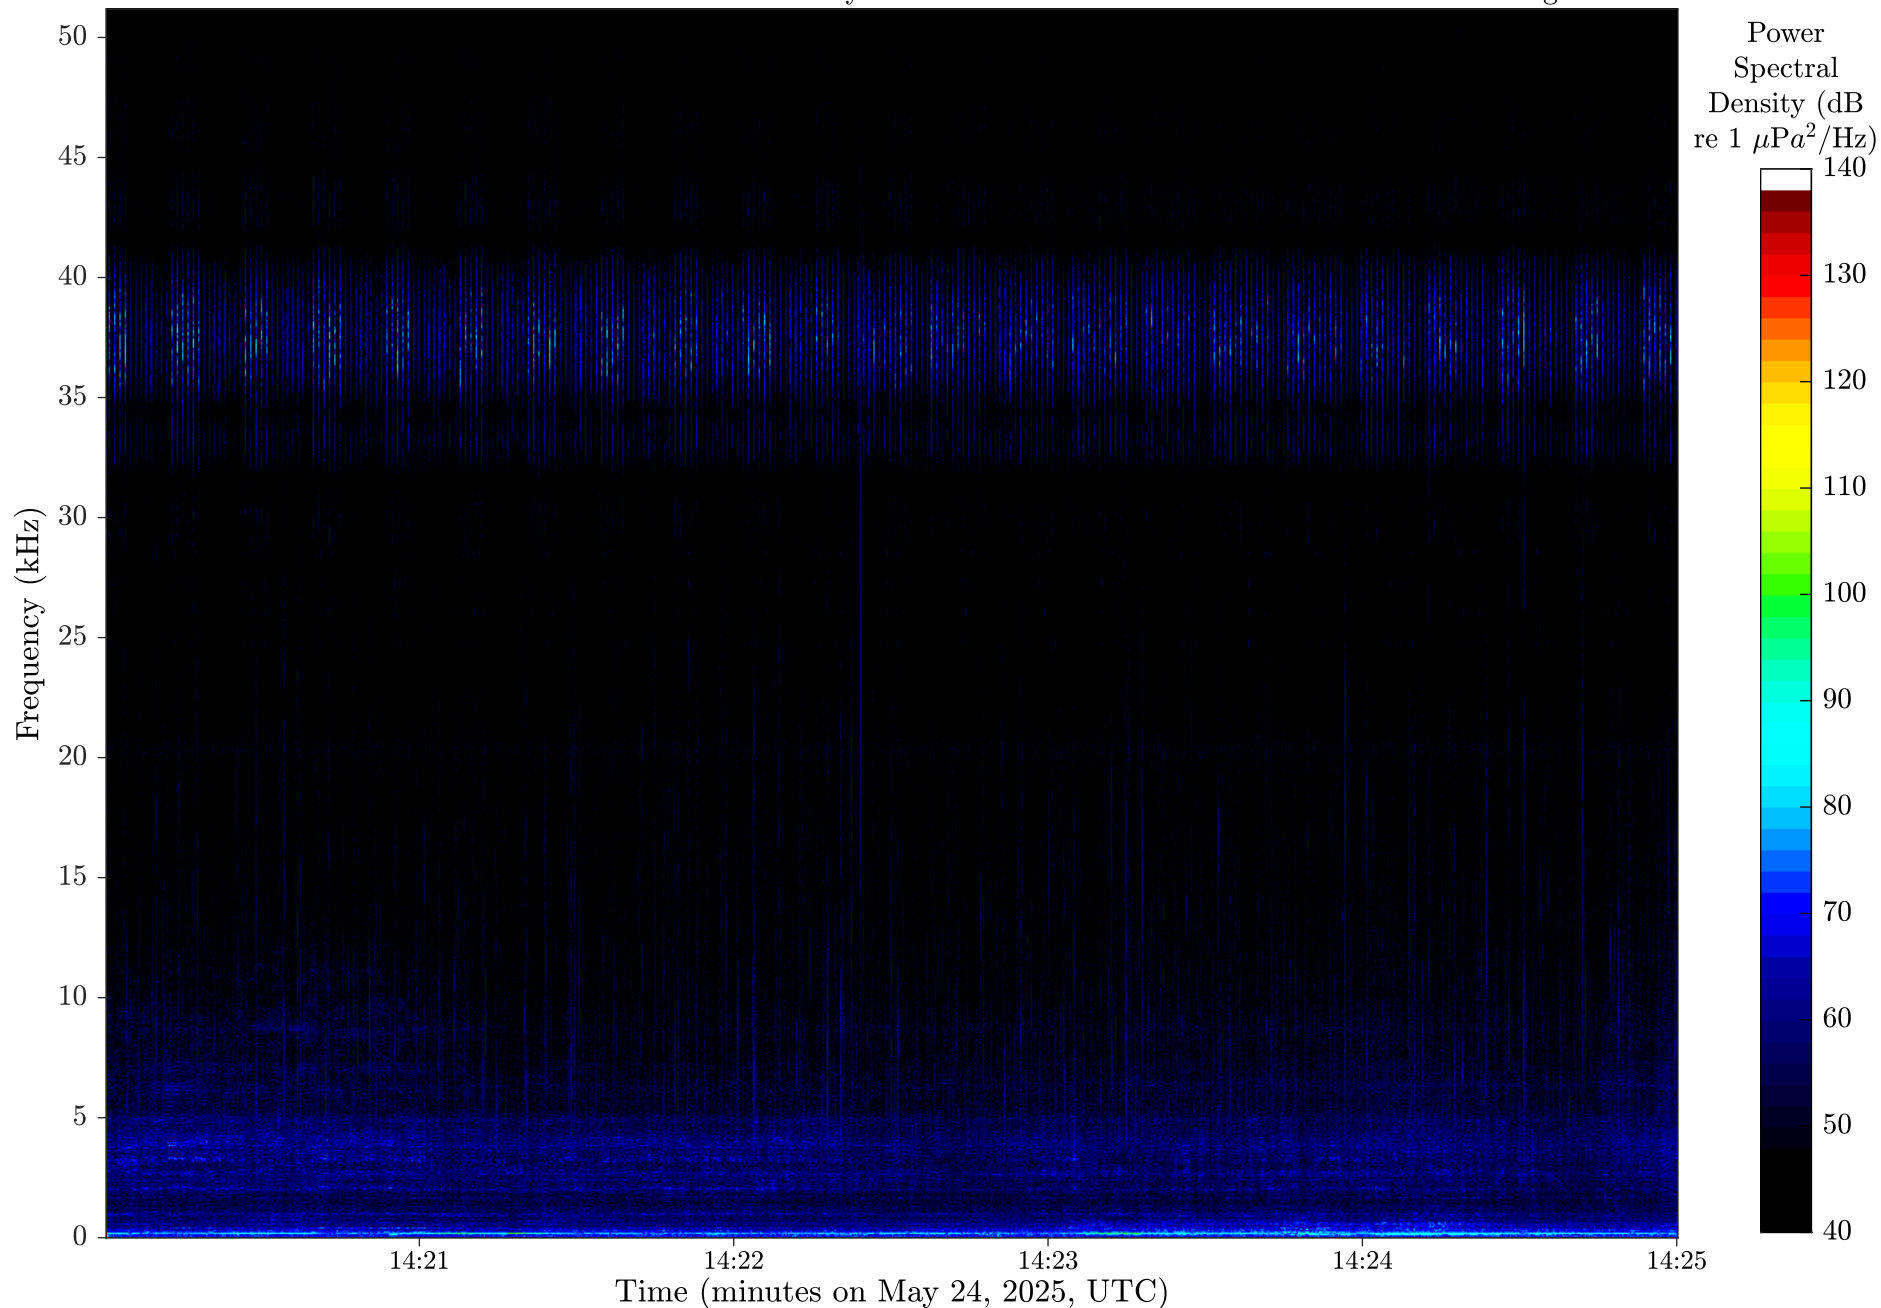


Comments: 30.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:32 UTC

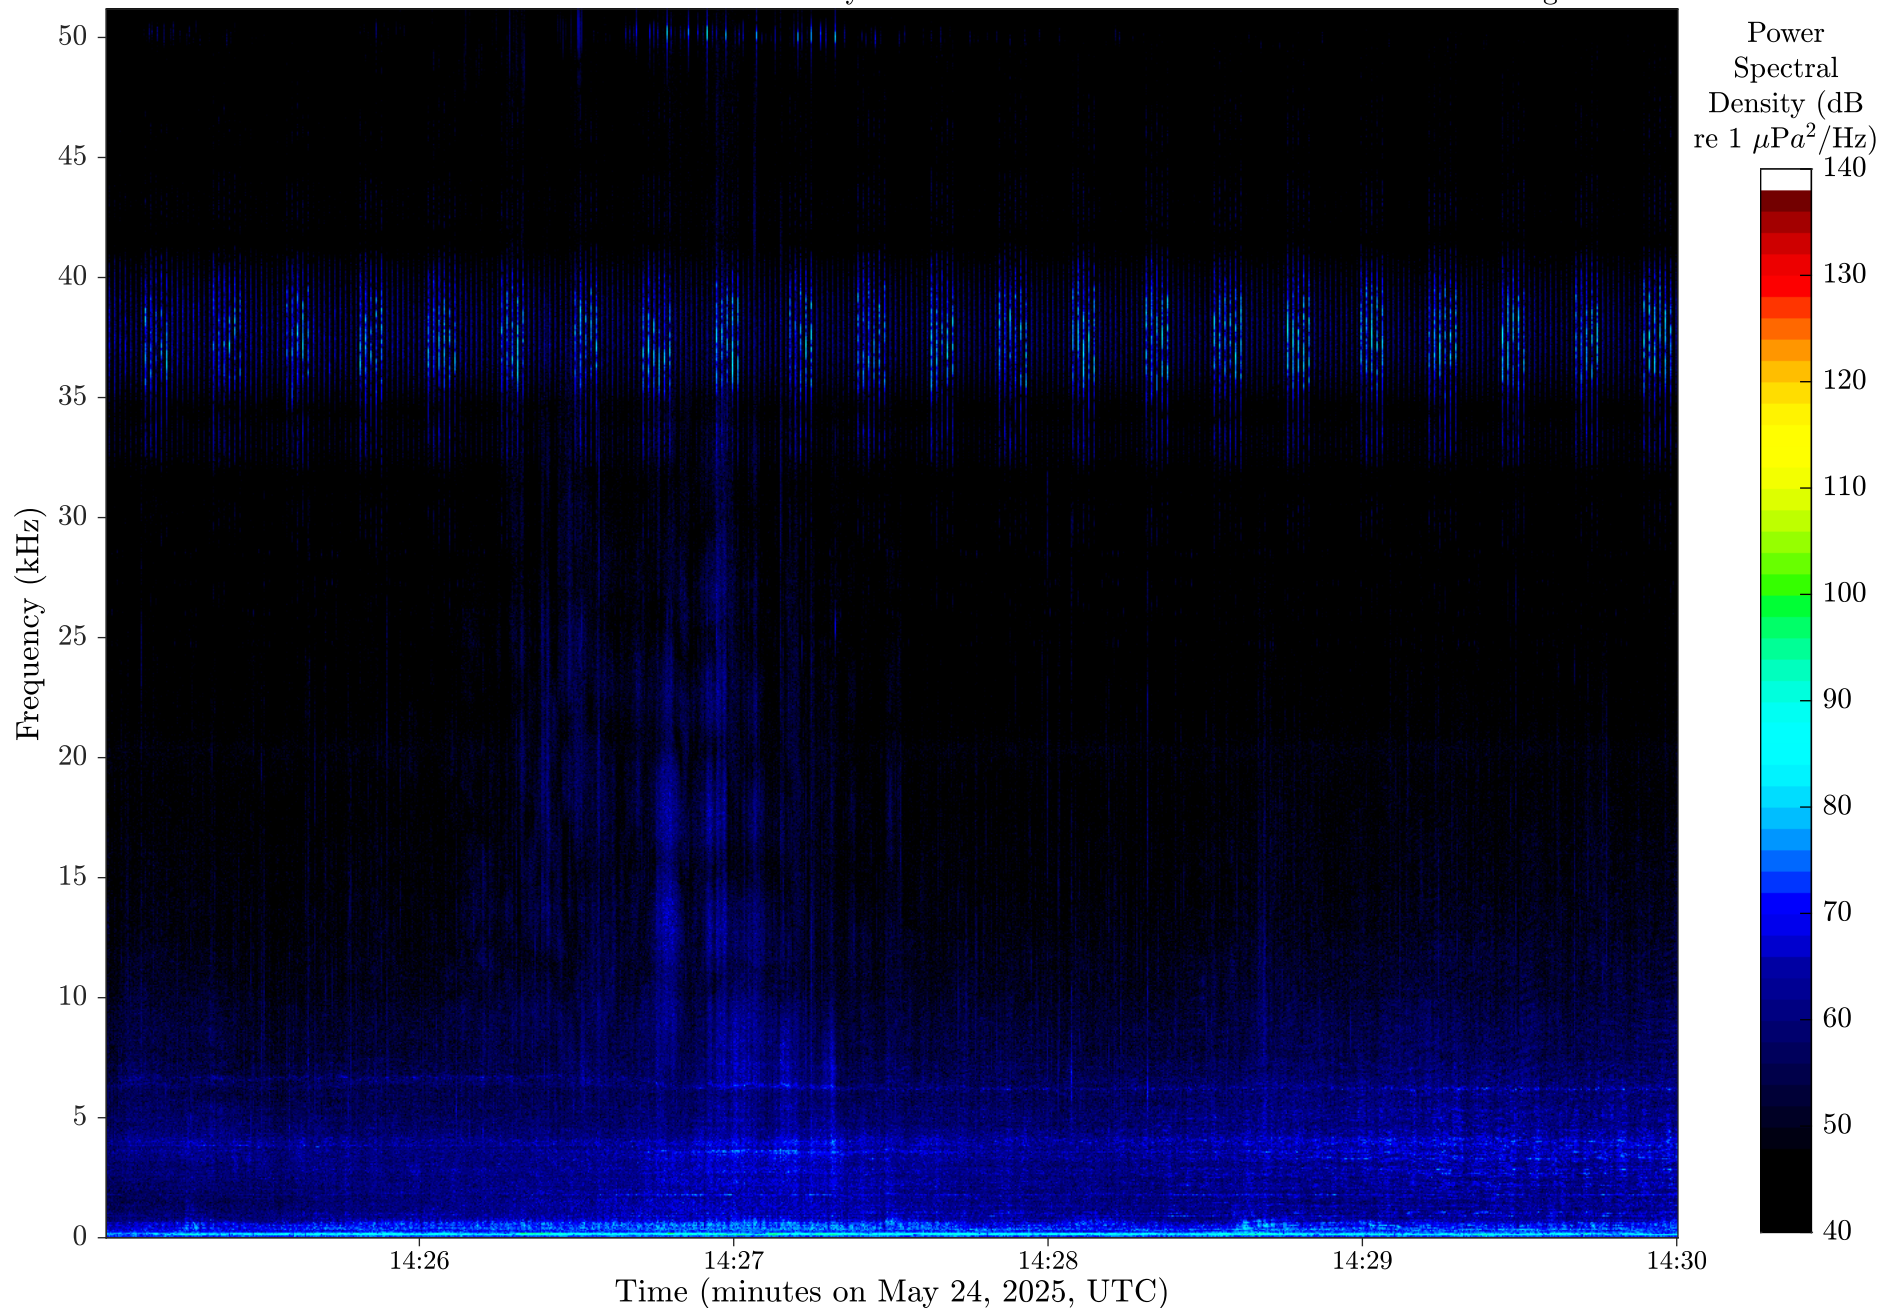


Comments: 20.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:40 UTC

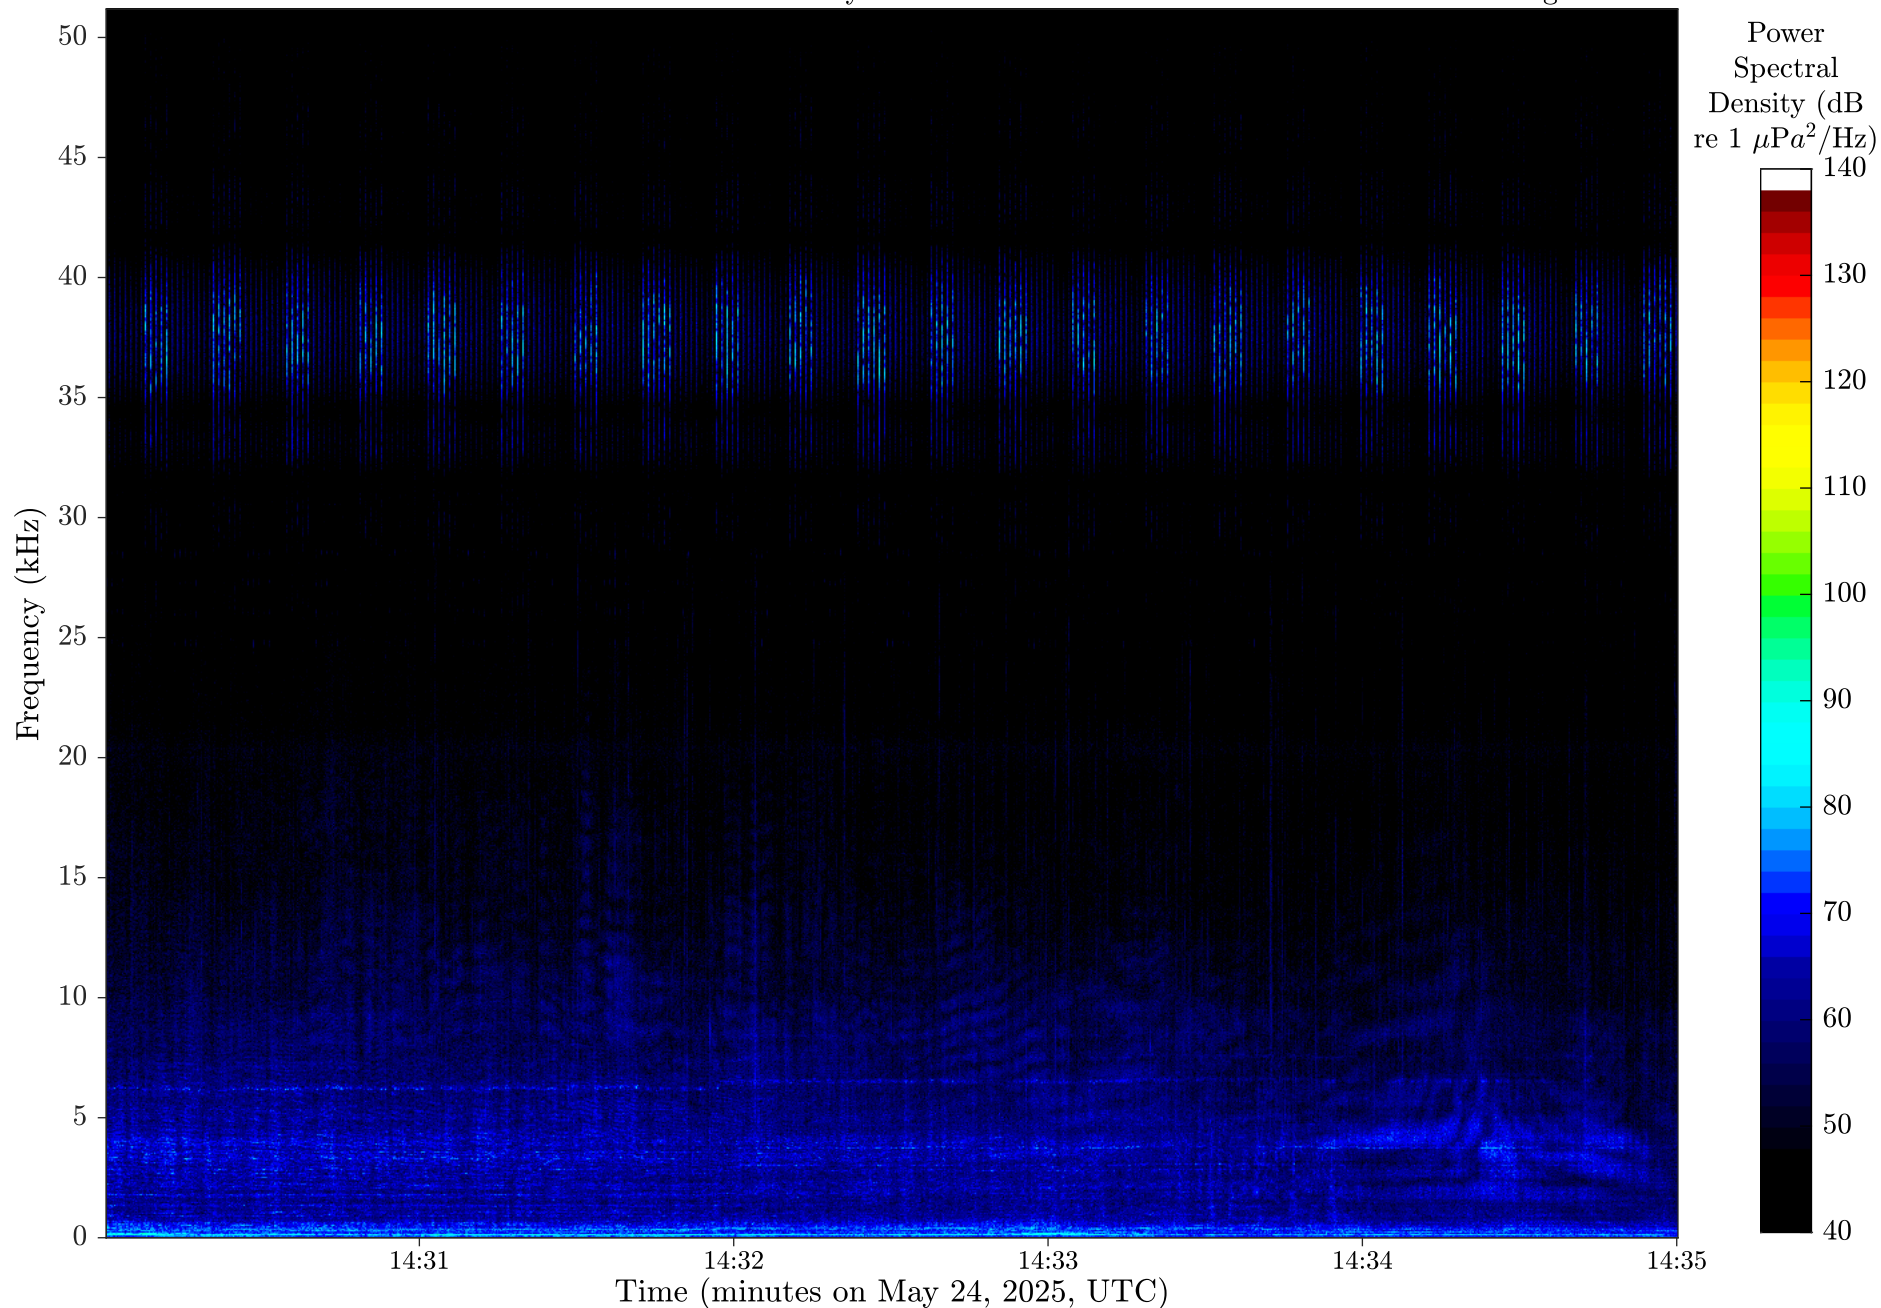


Comments: 27.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:42:48 UTC

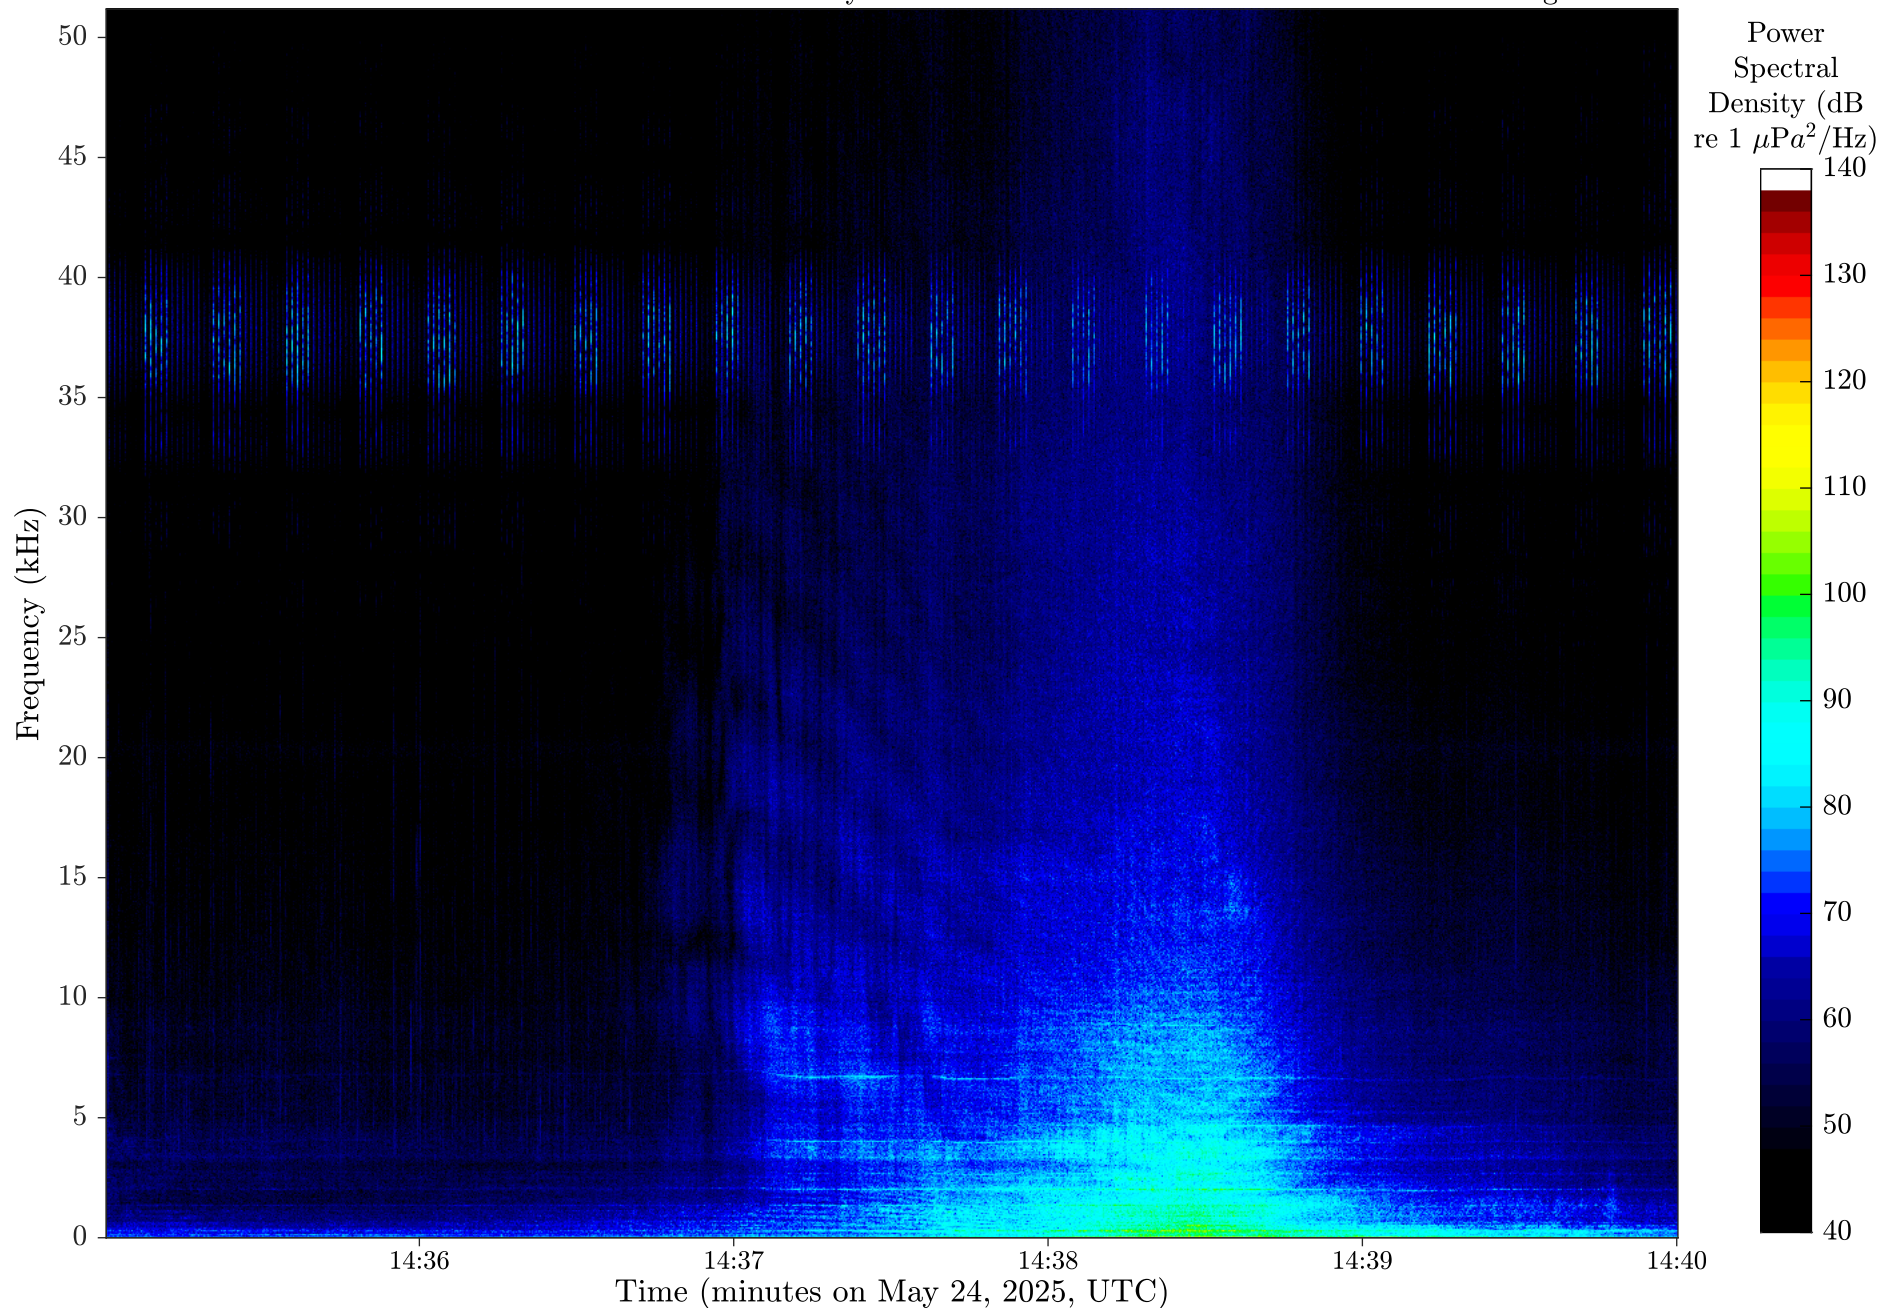


Comments: 15 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:42:56 UTC

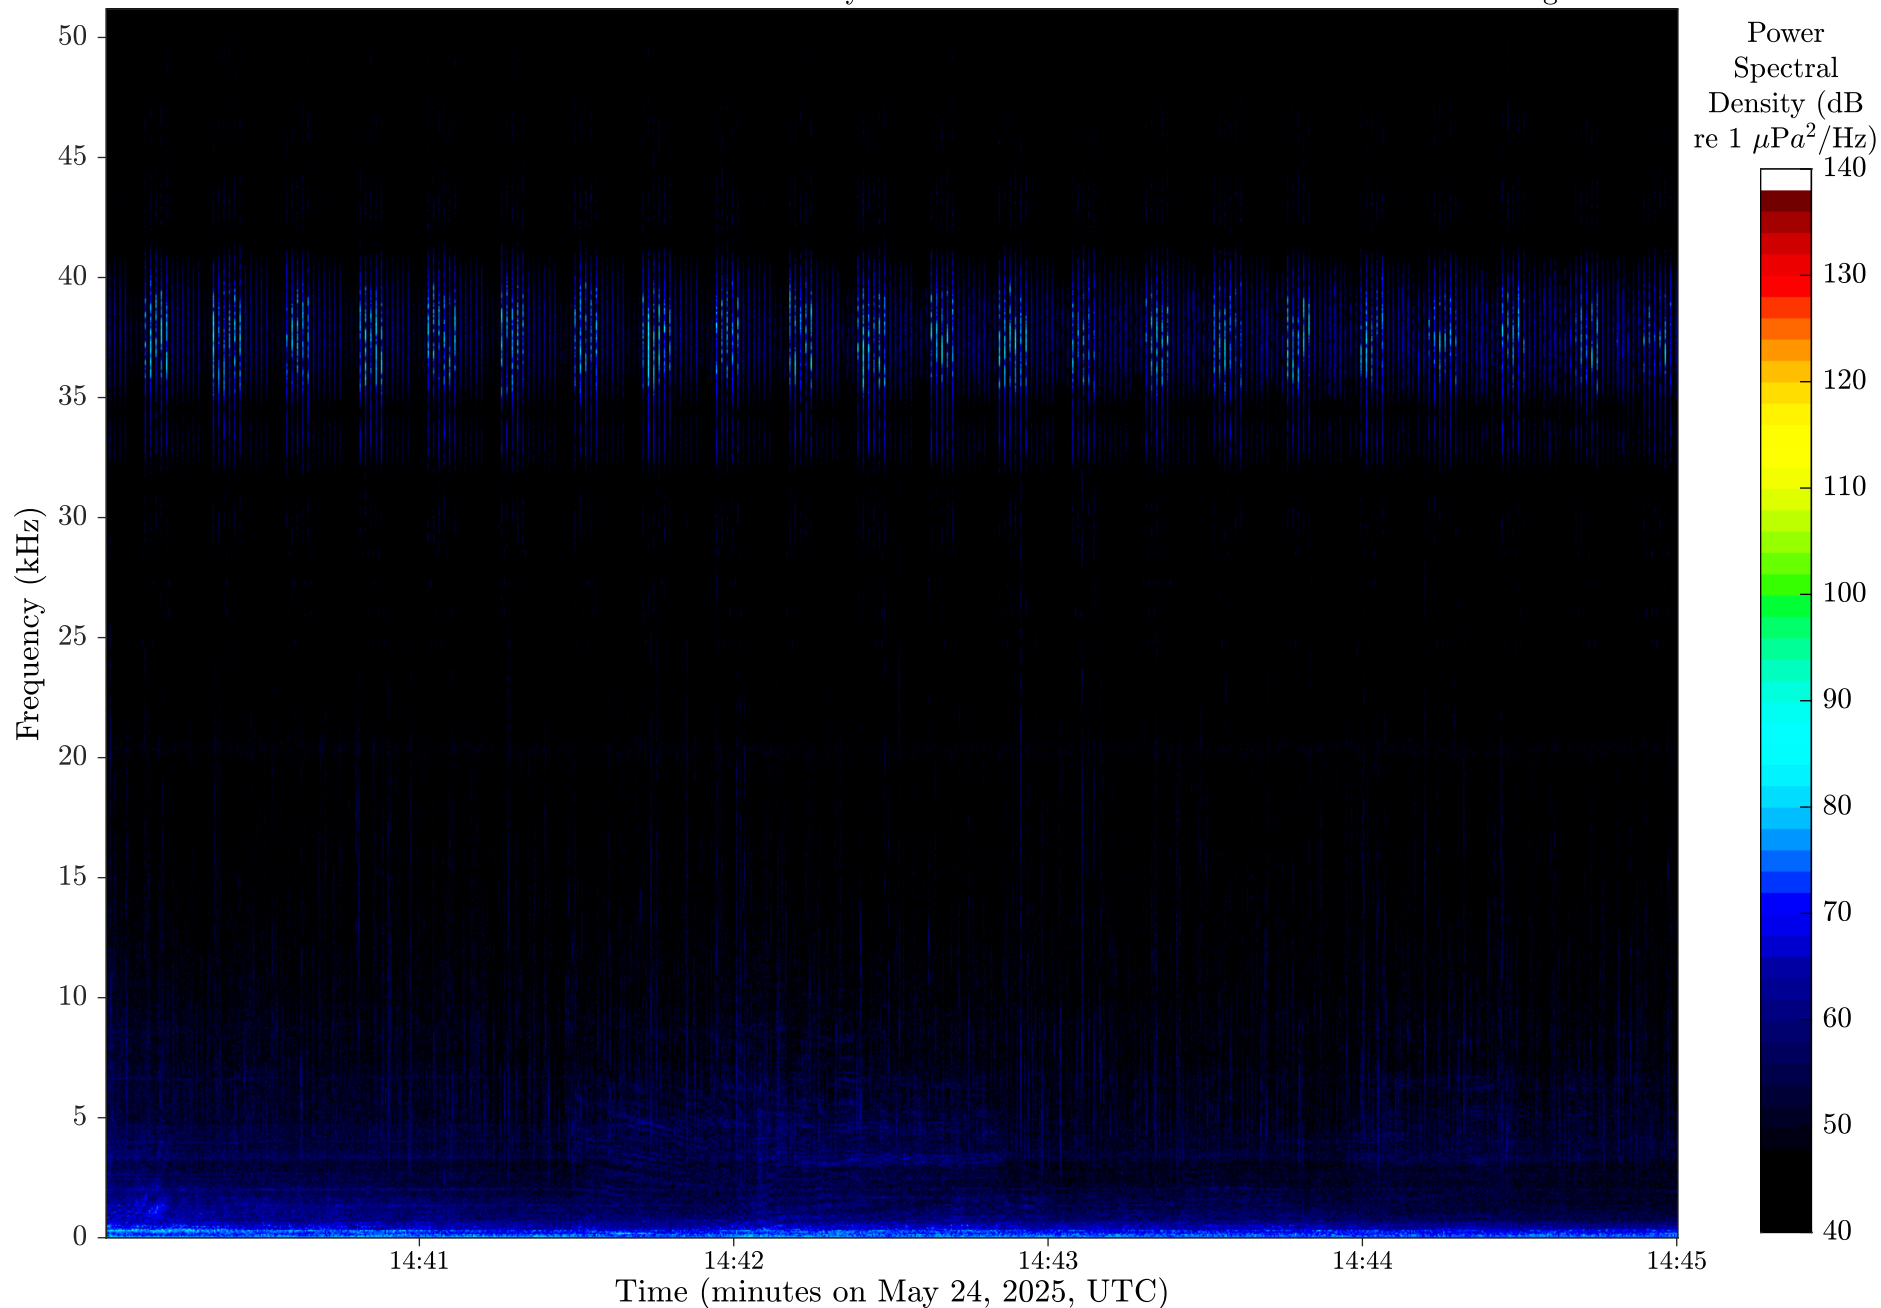

Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:43:03 UTC

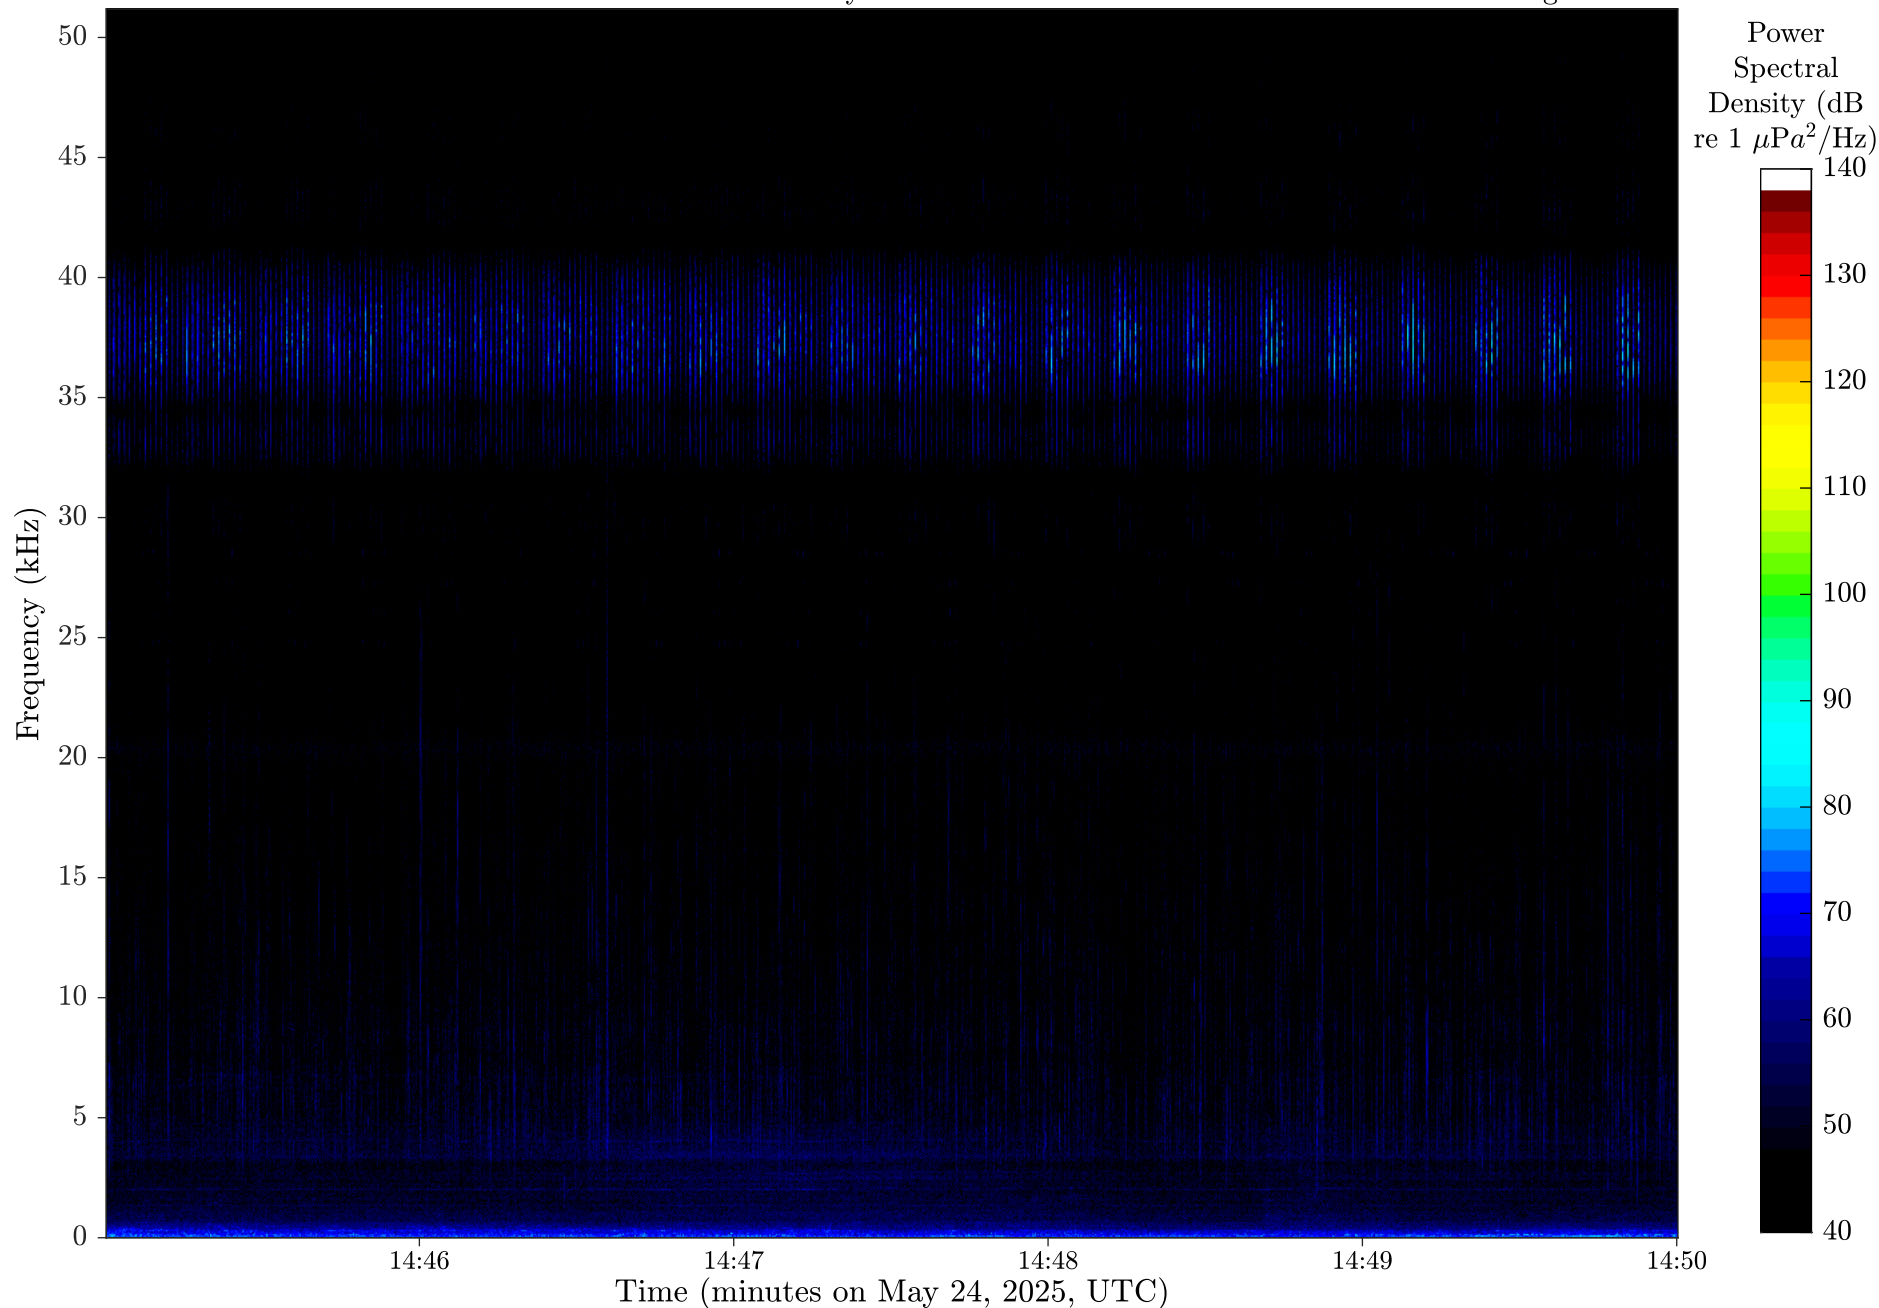


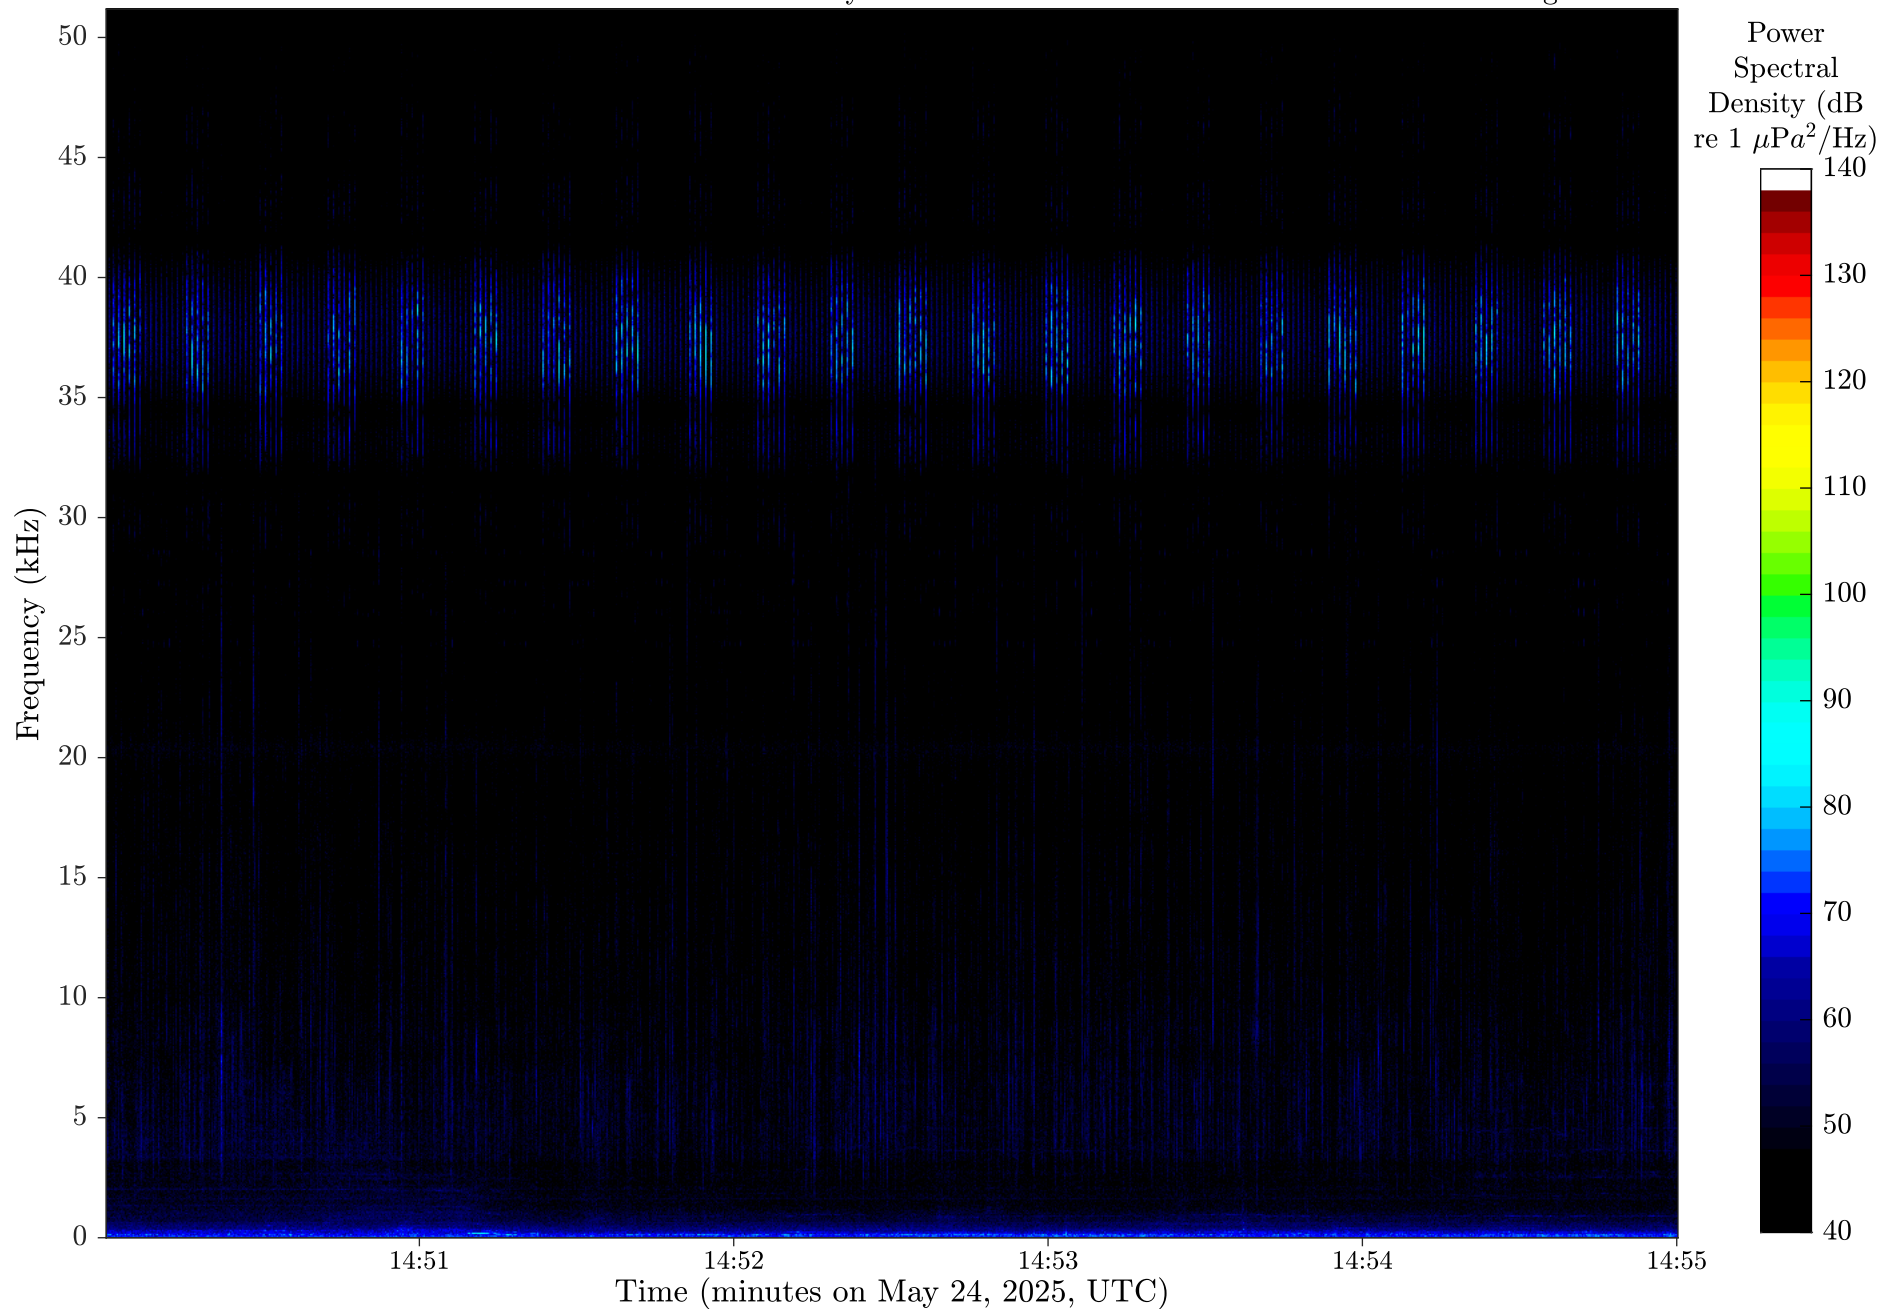

Comments: 32 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:43:19 UTC

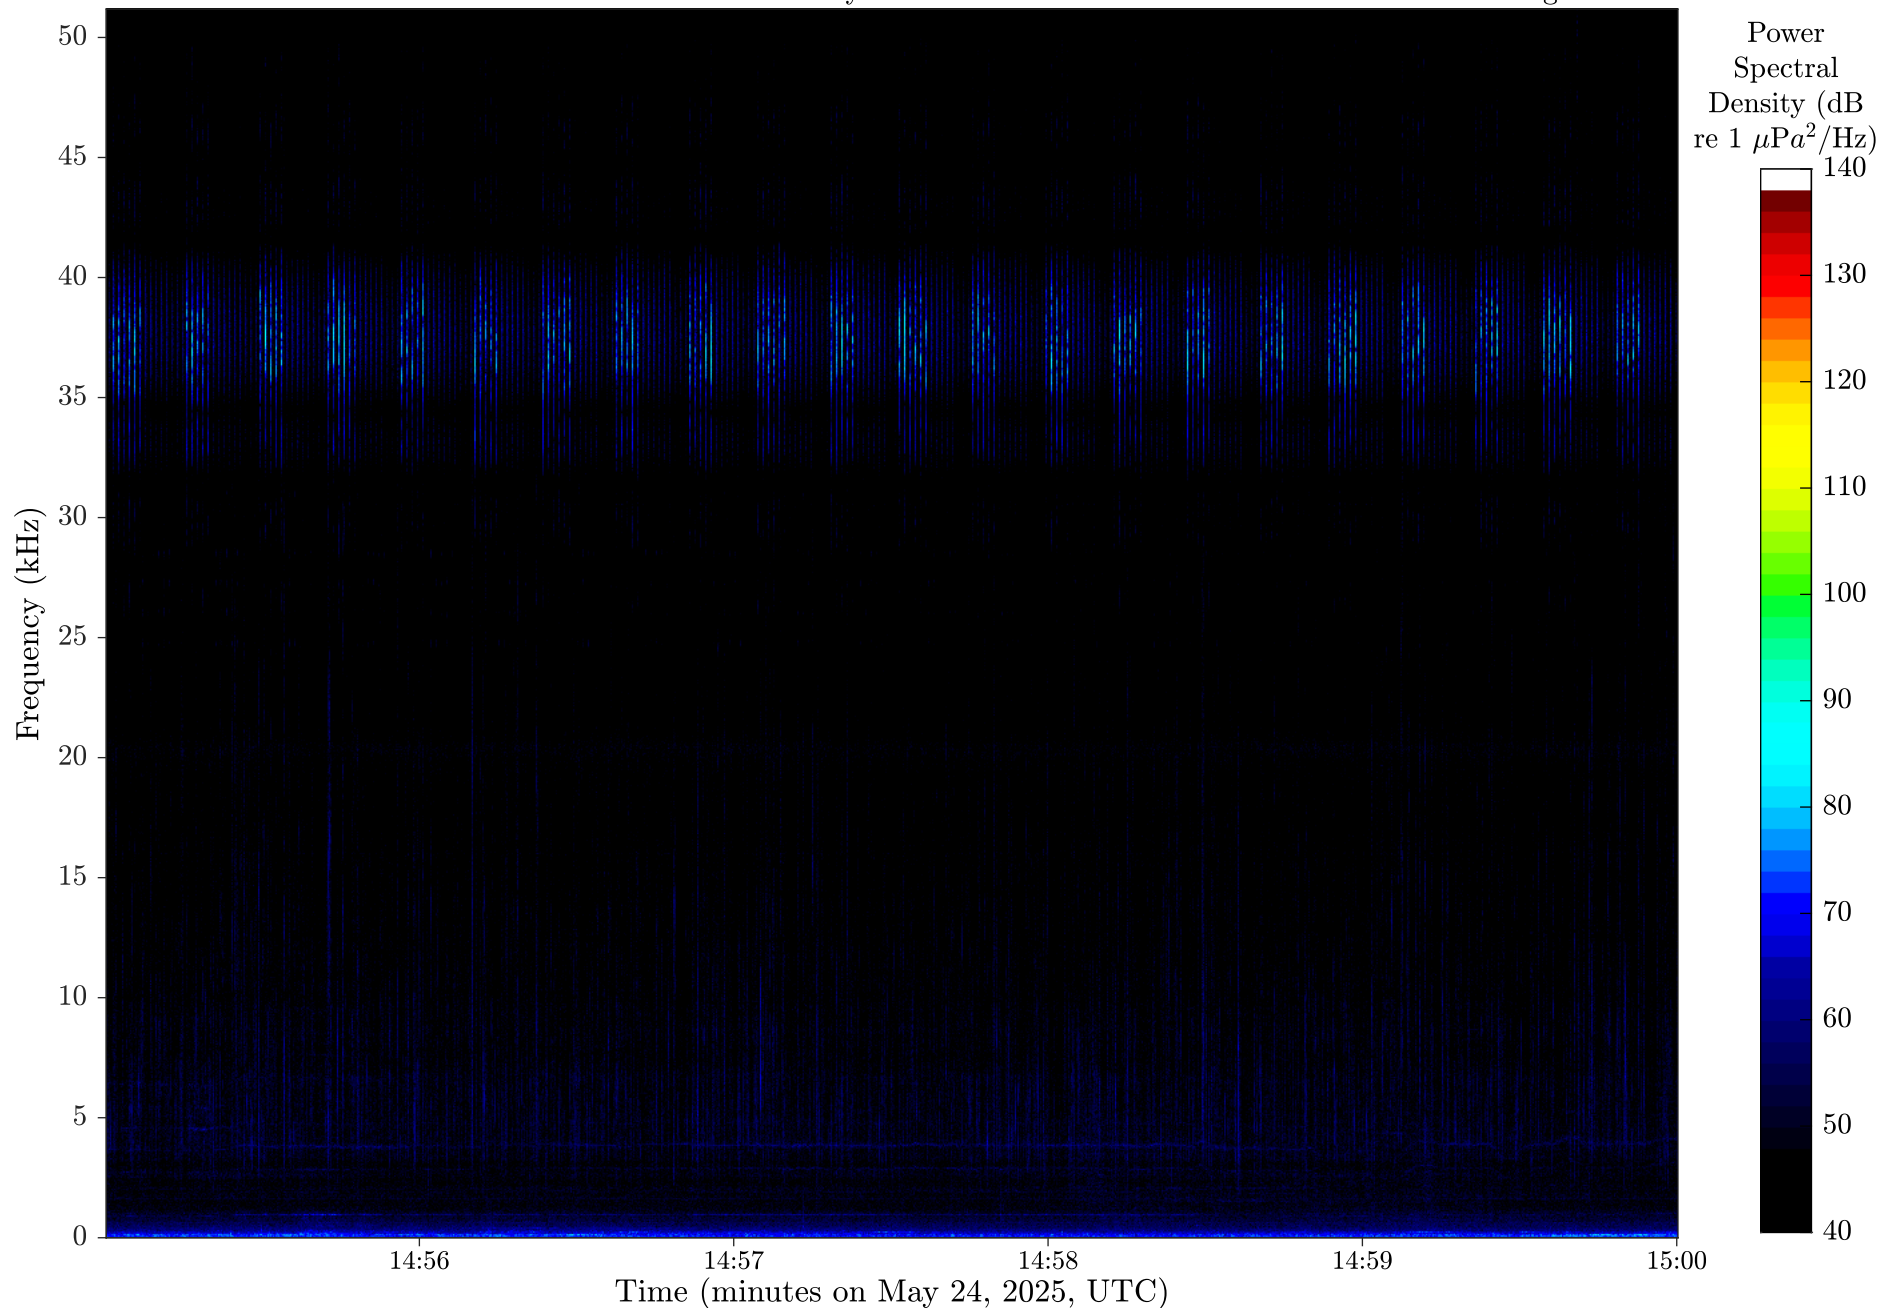

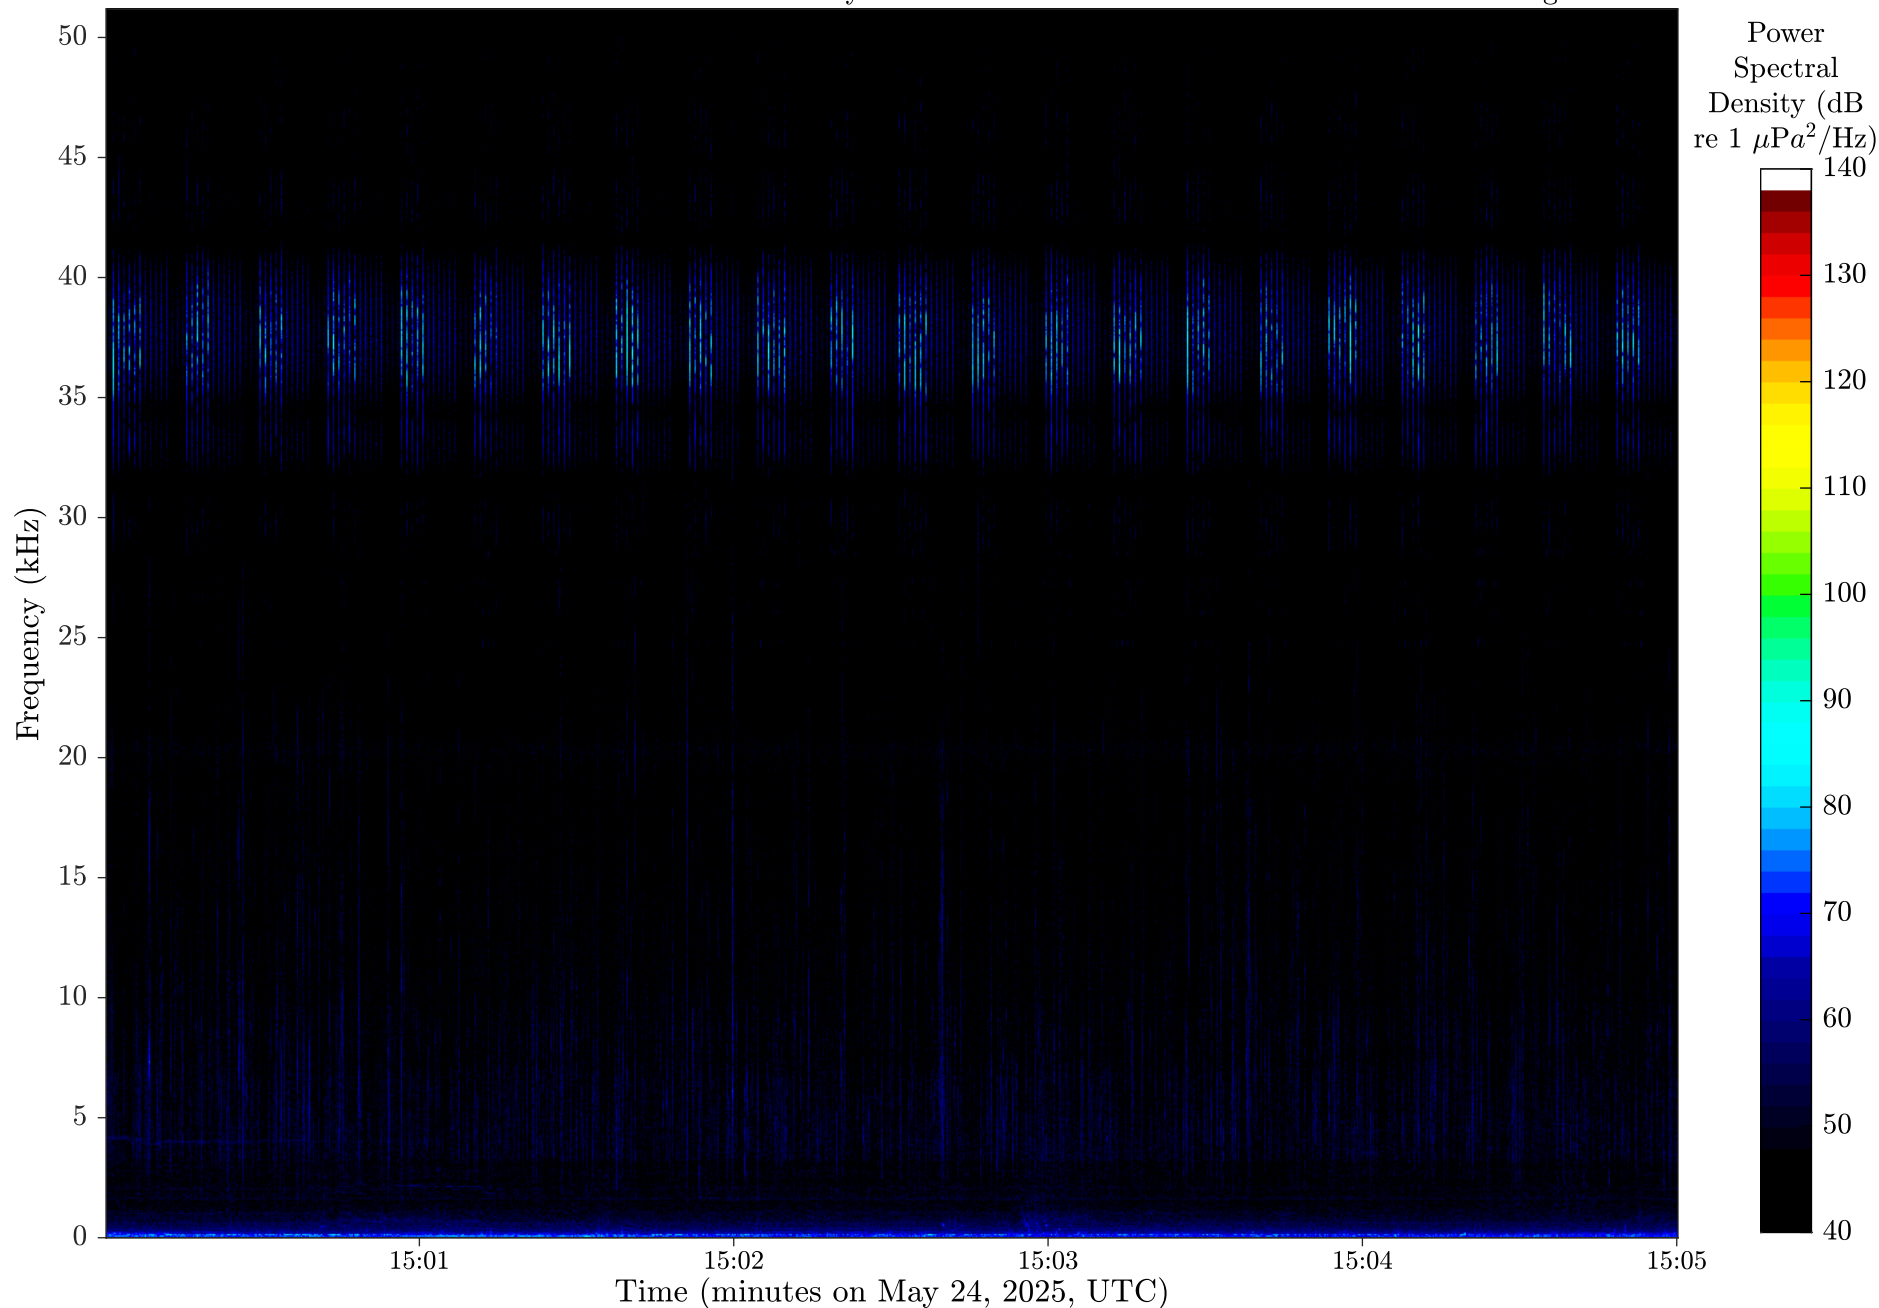


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:43:35 UTC

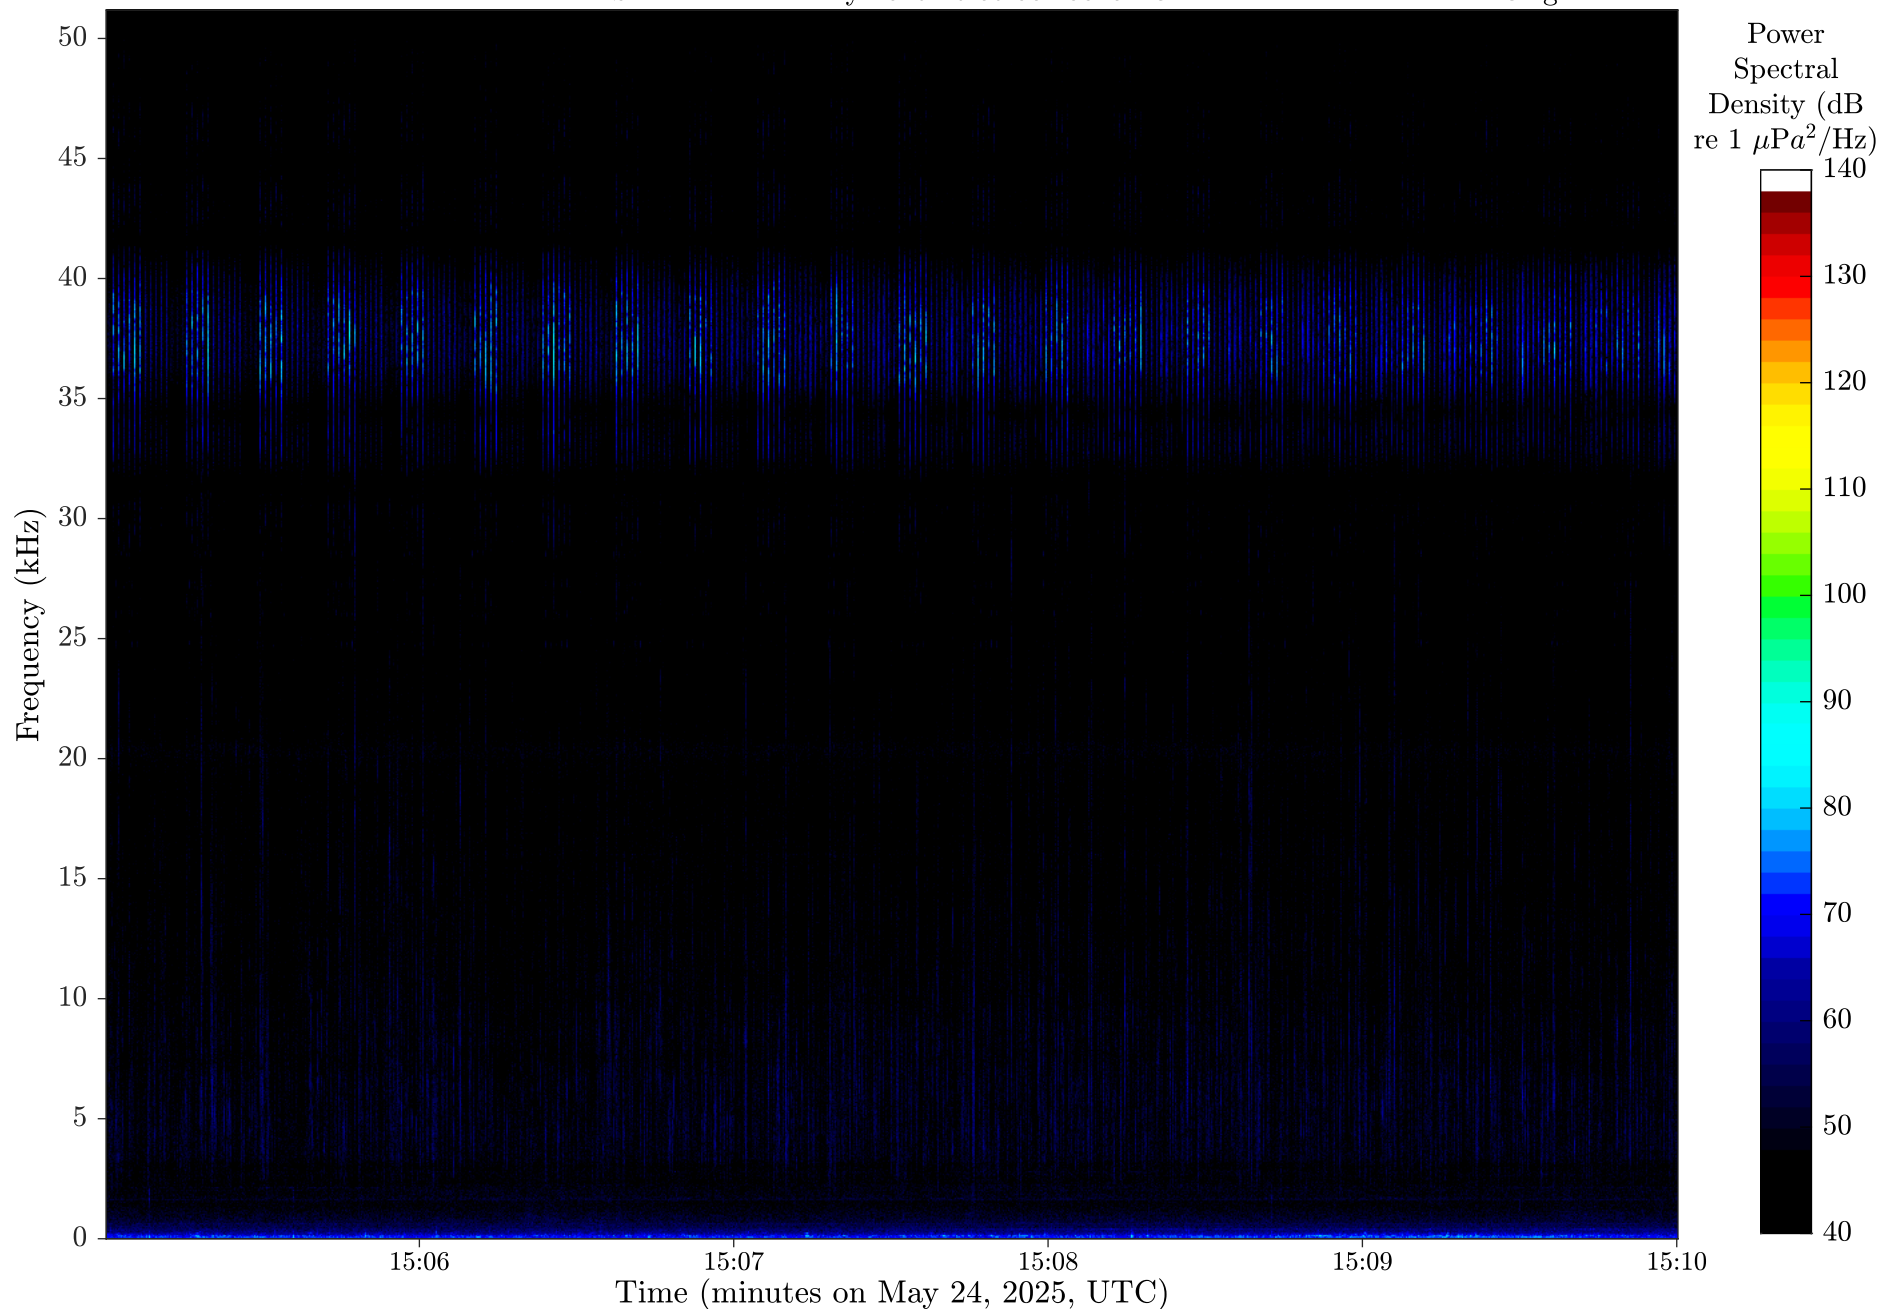


Comments: 32.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:43:42 UTC

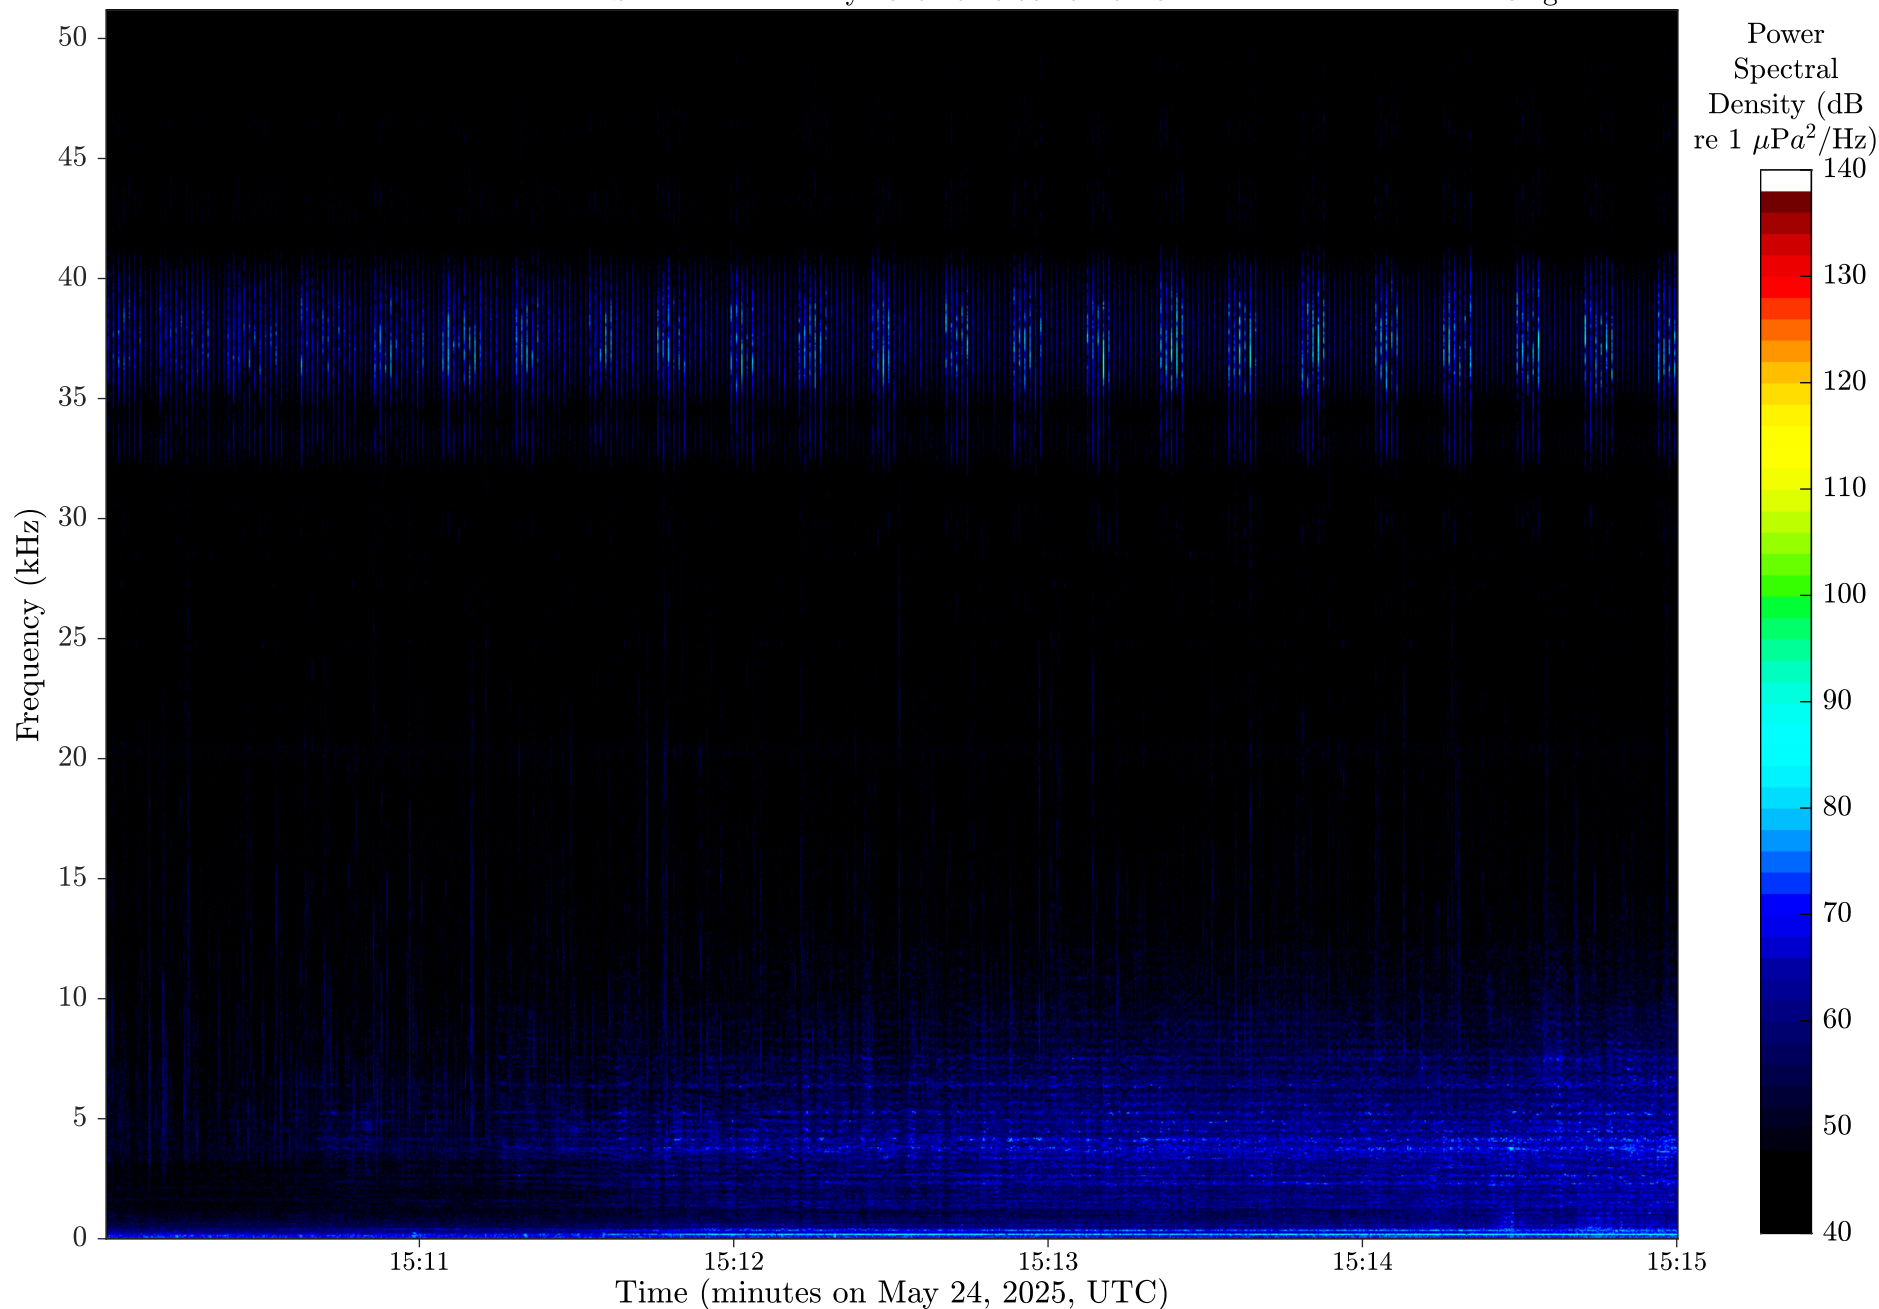


Comments: 31.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:43:50 UTC

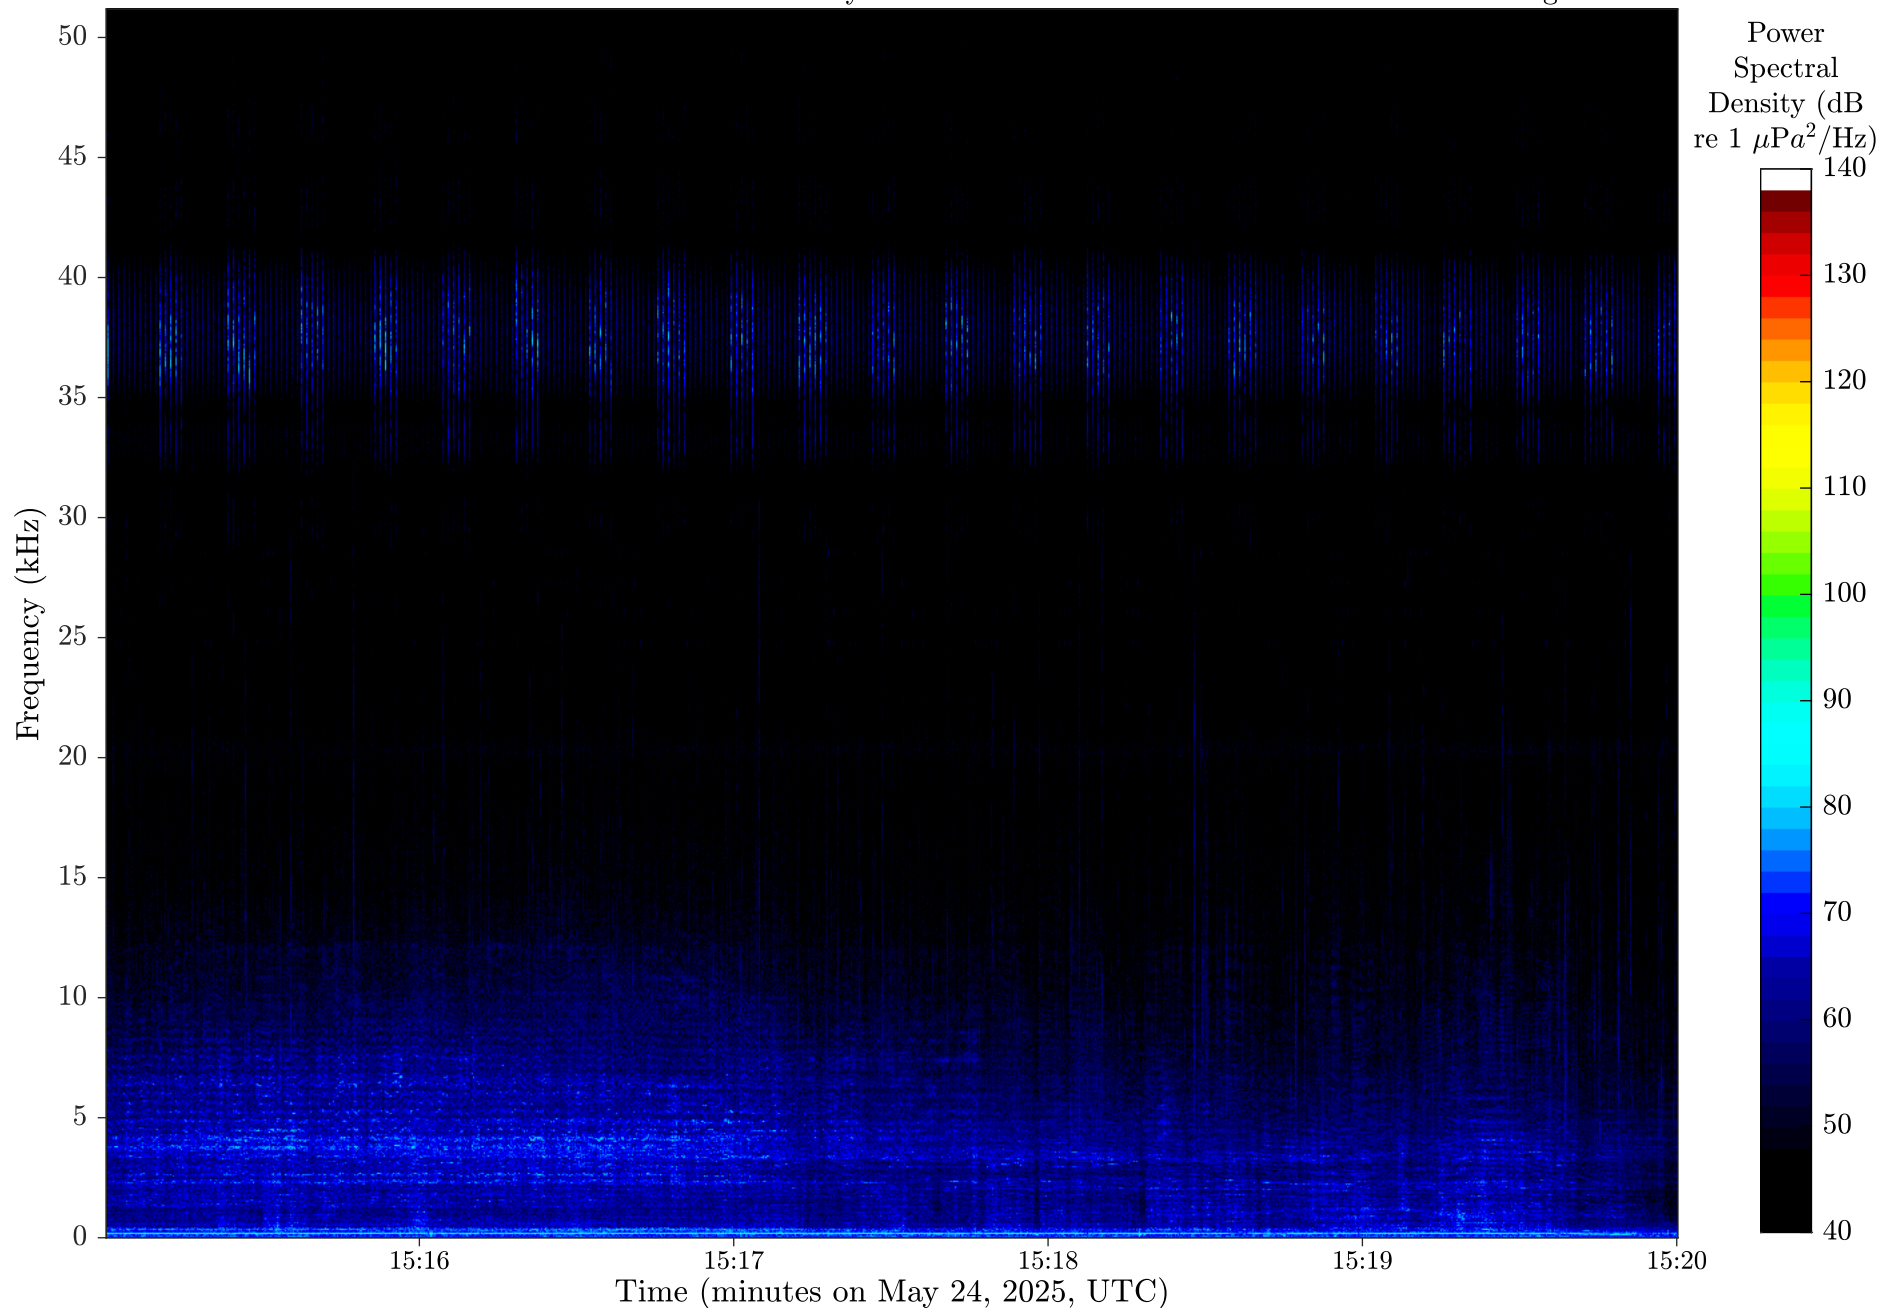


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:43:58 UTC

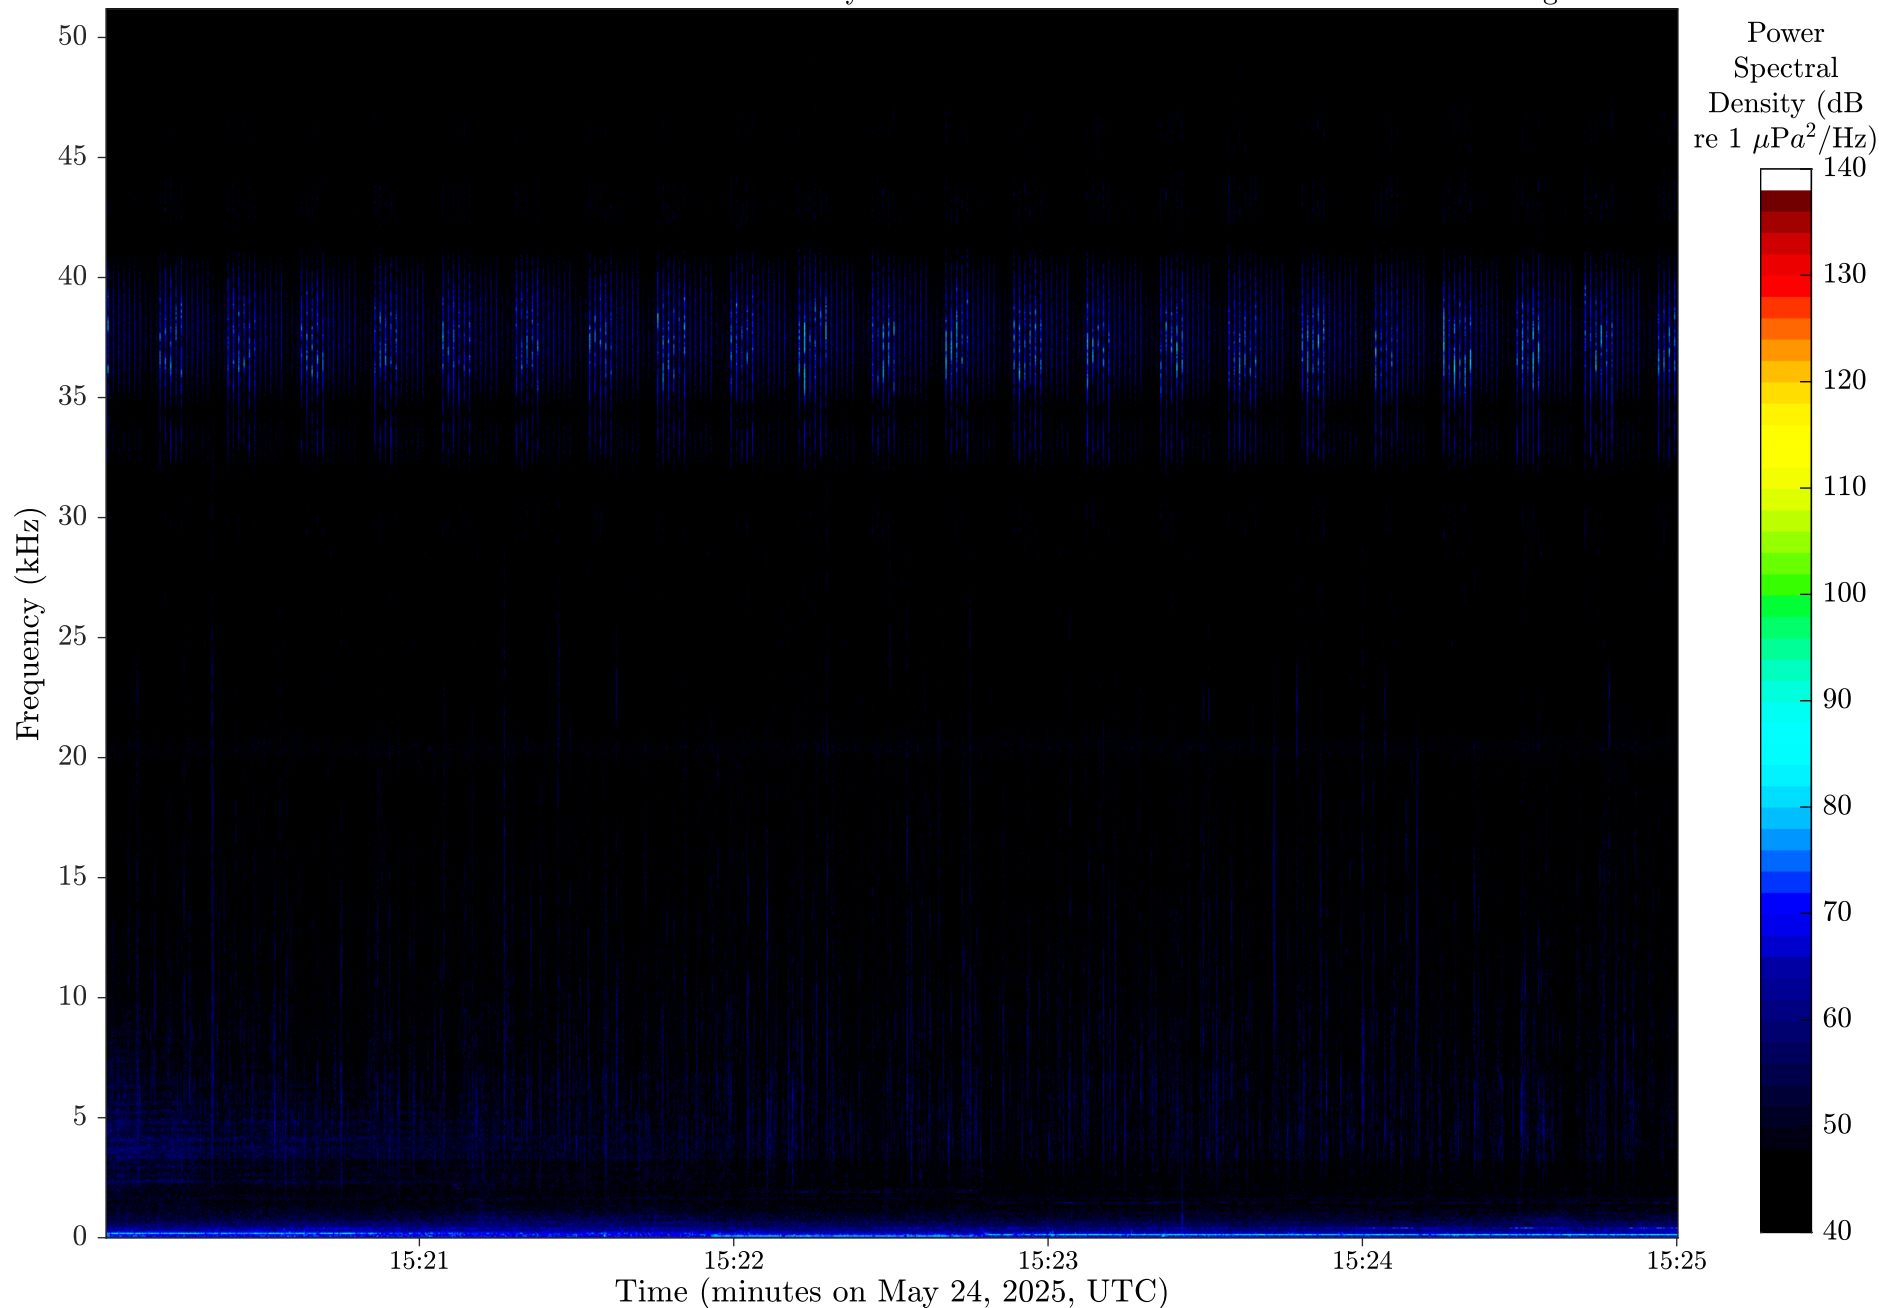


Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:44:05 UTC

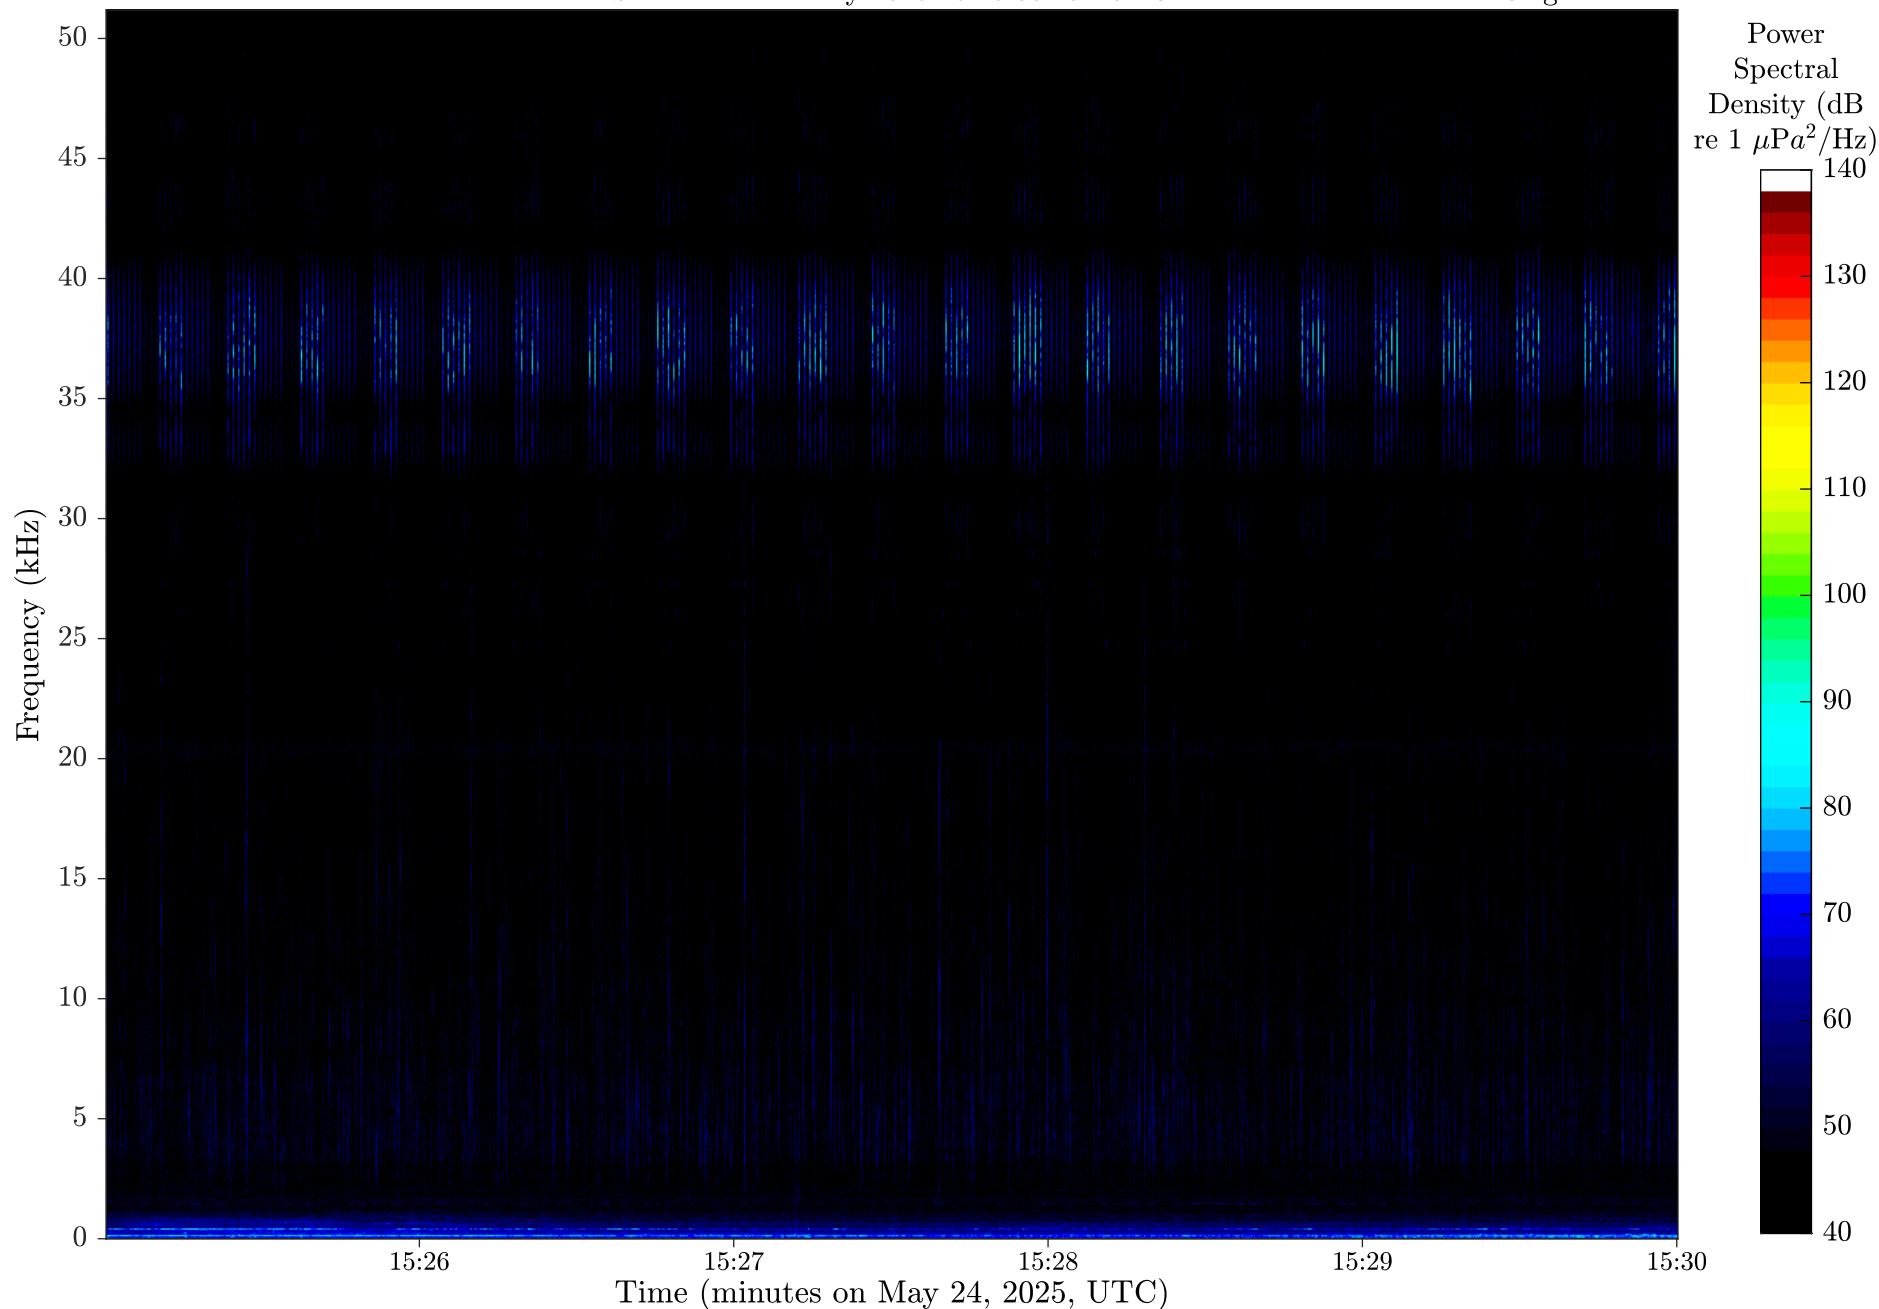



Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:13 UTC

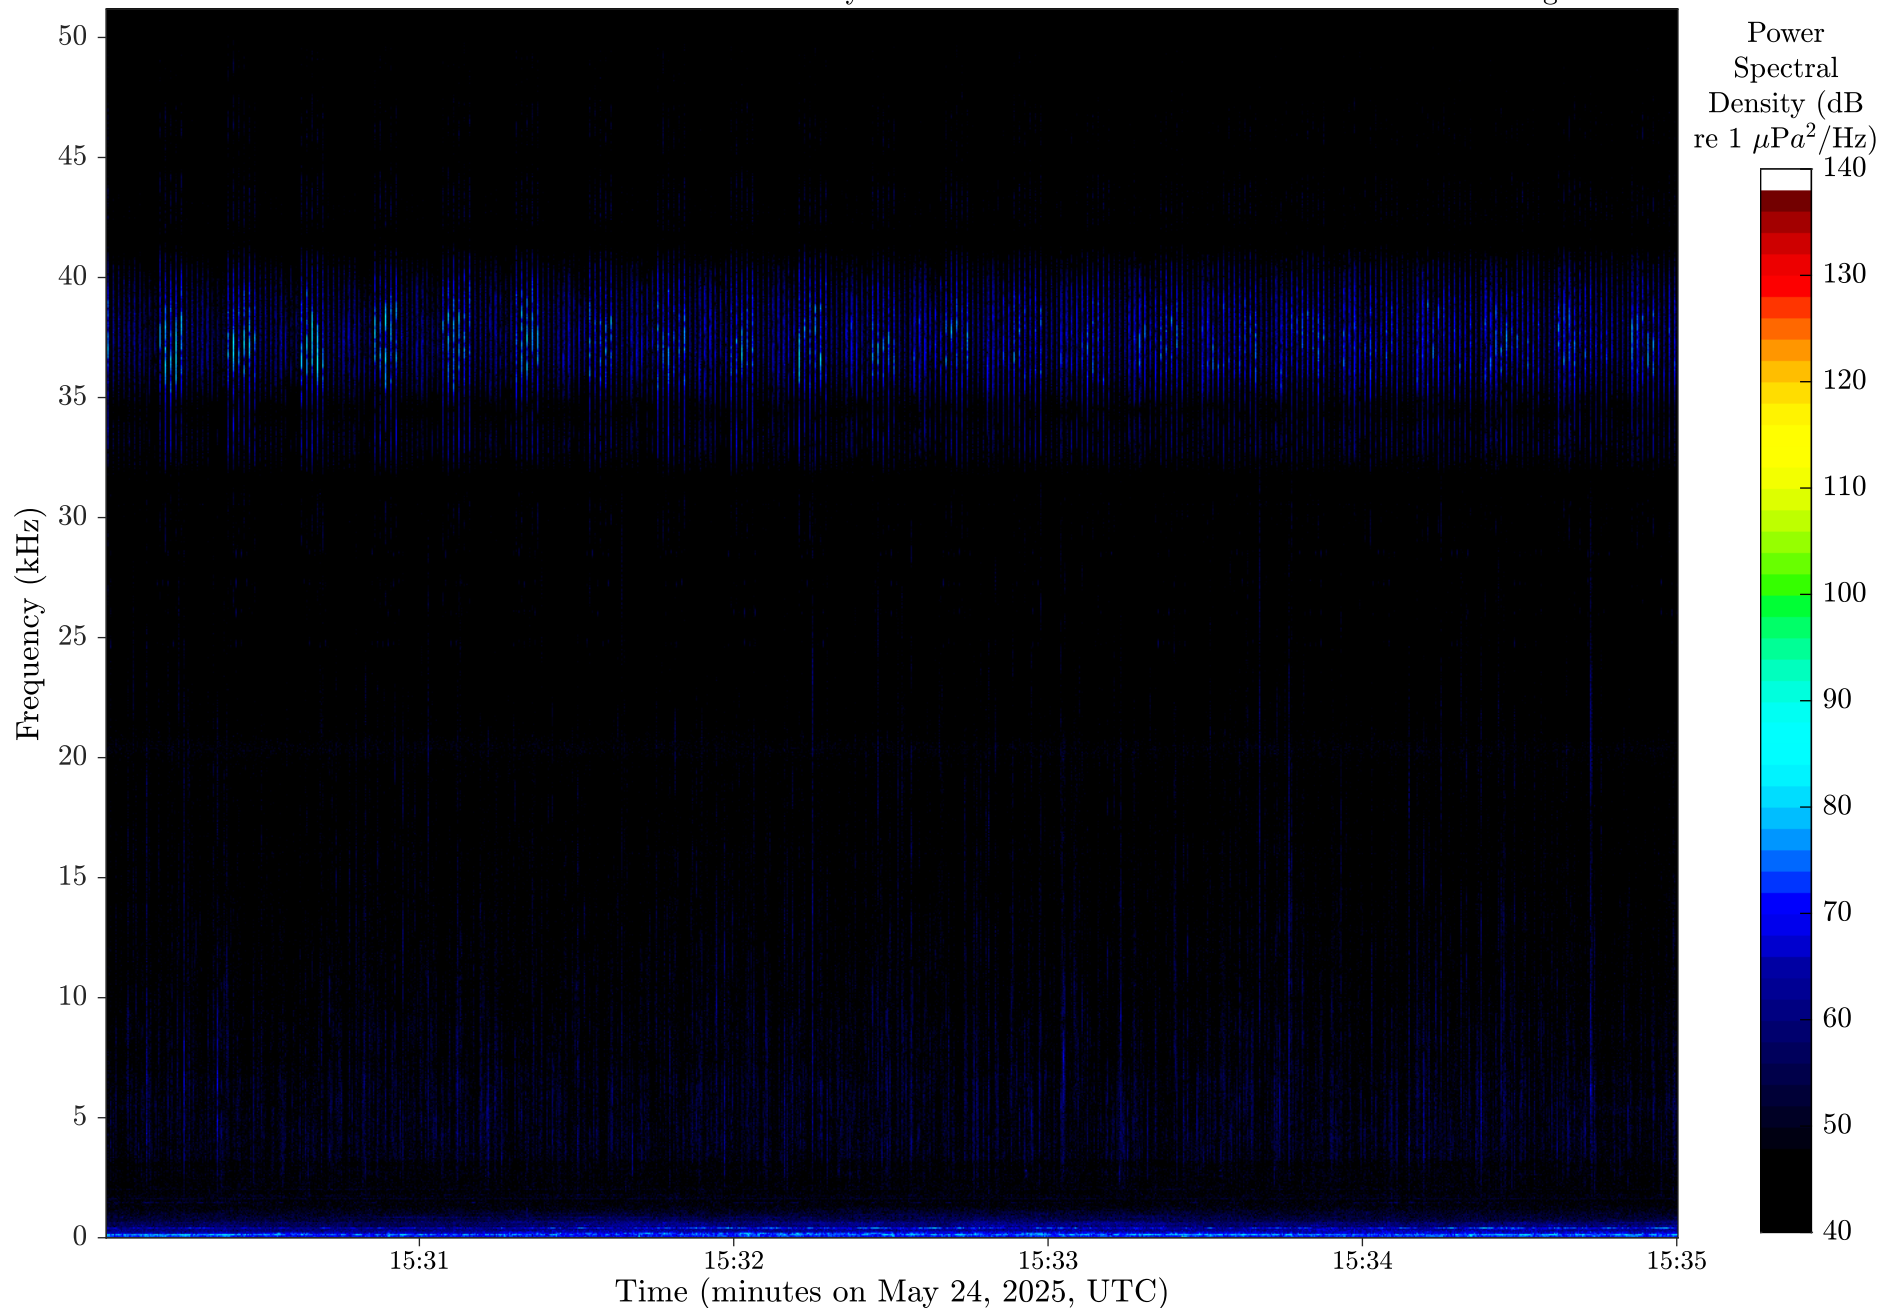

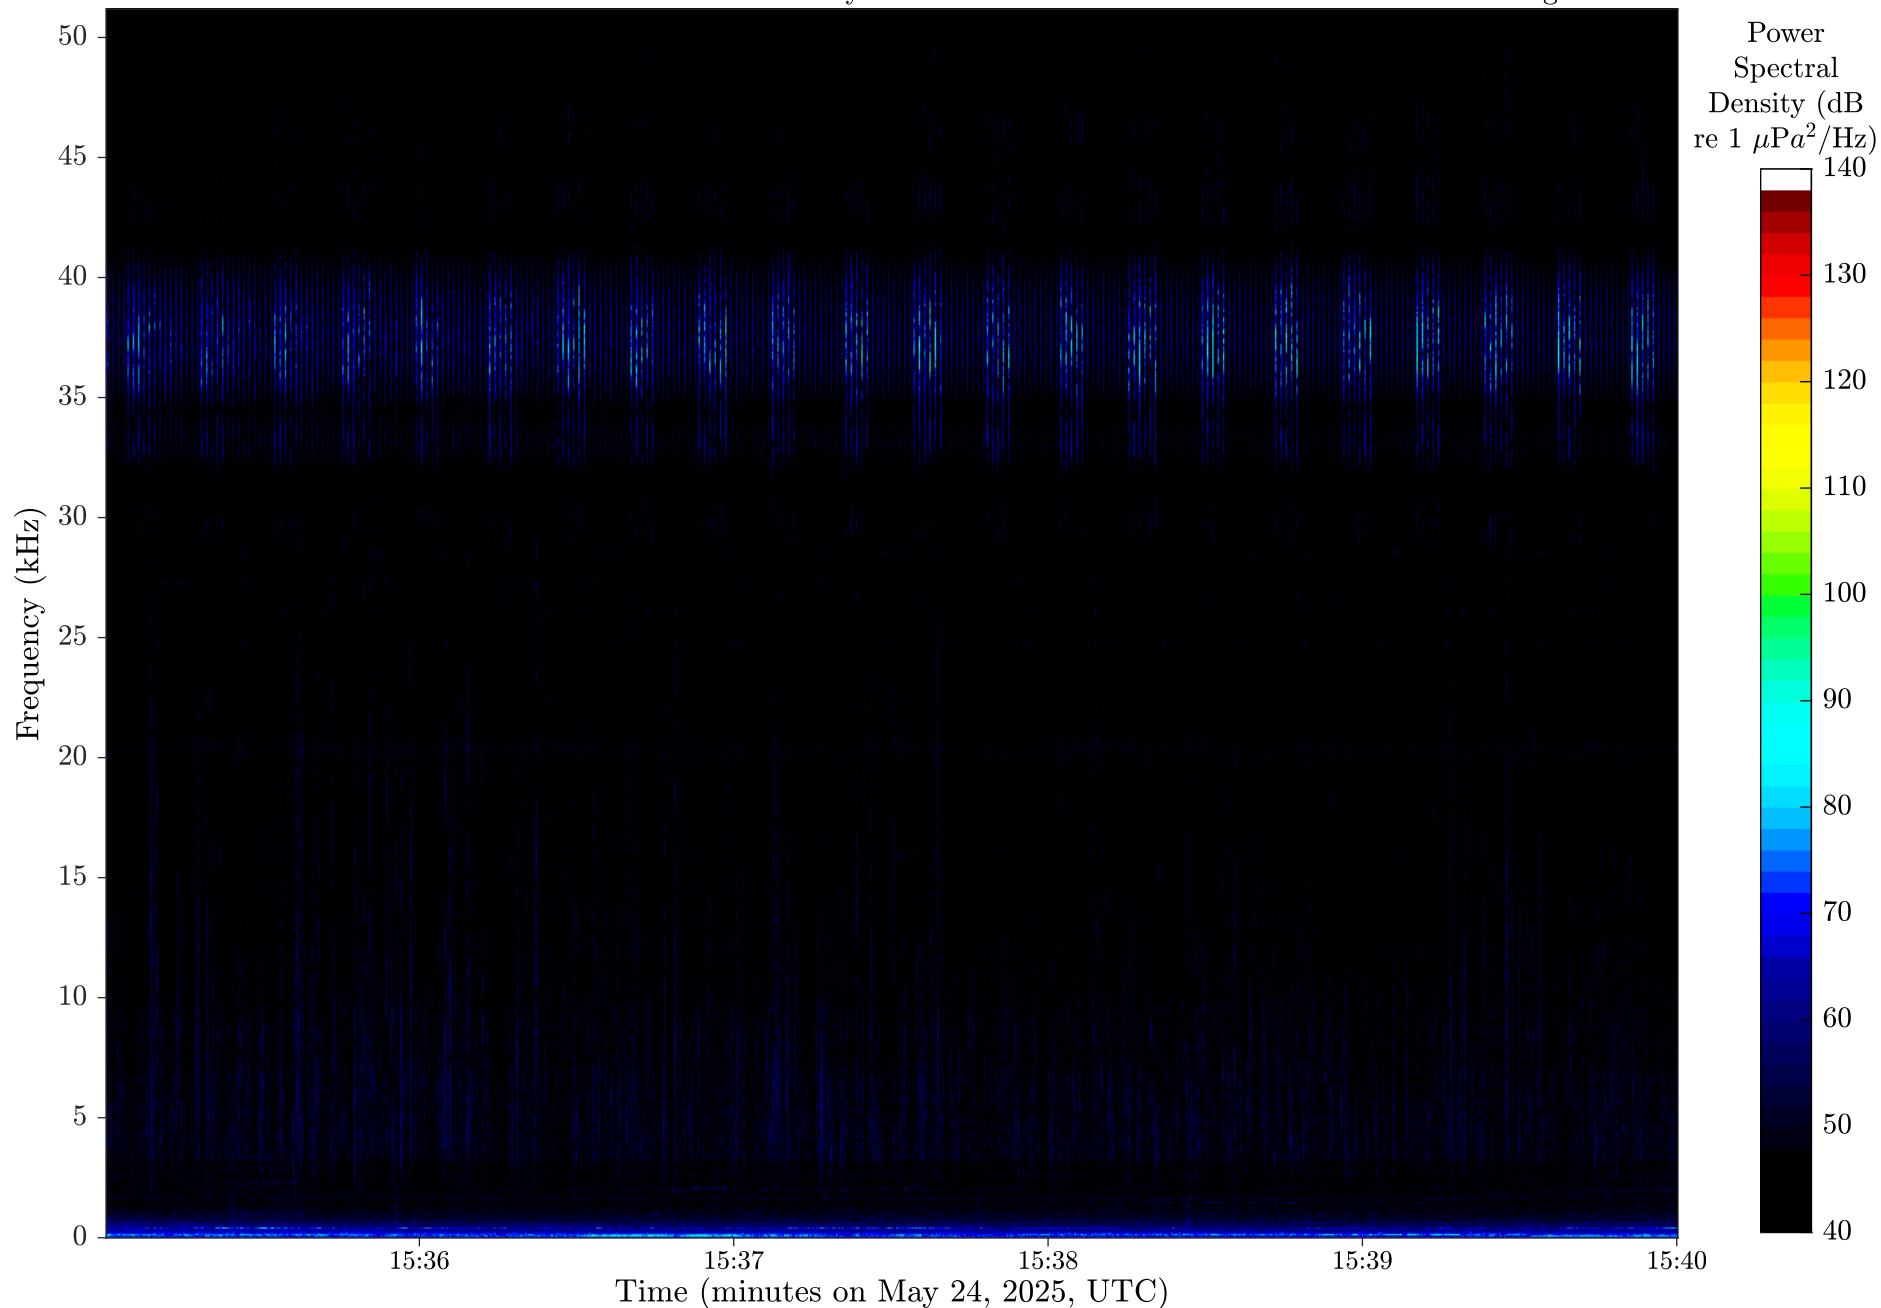


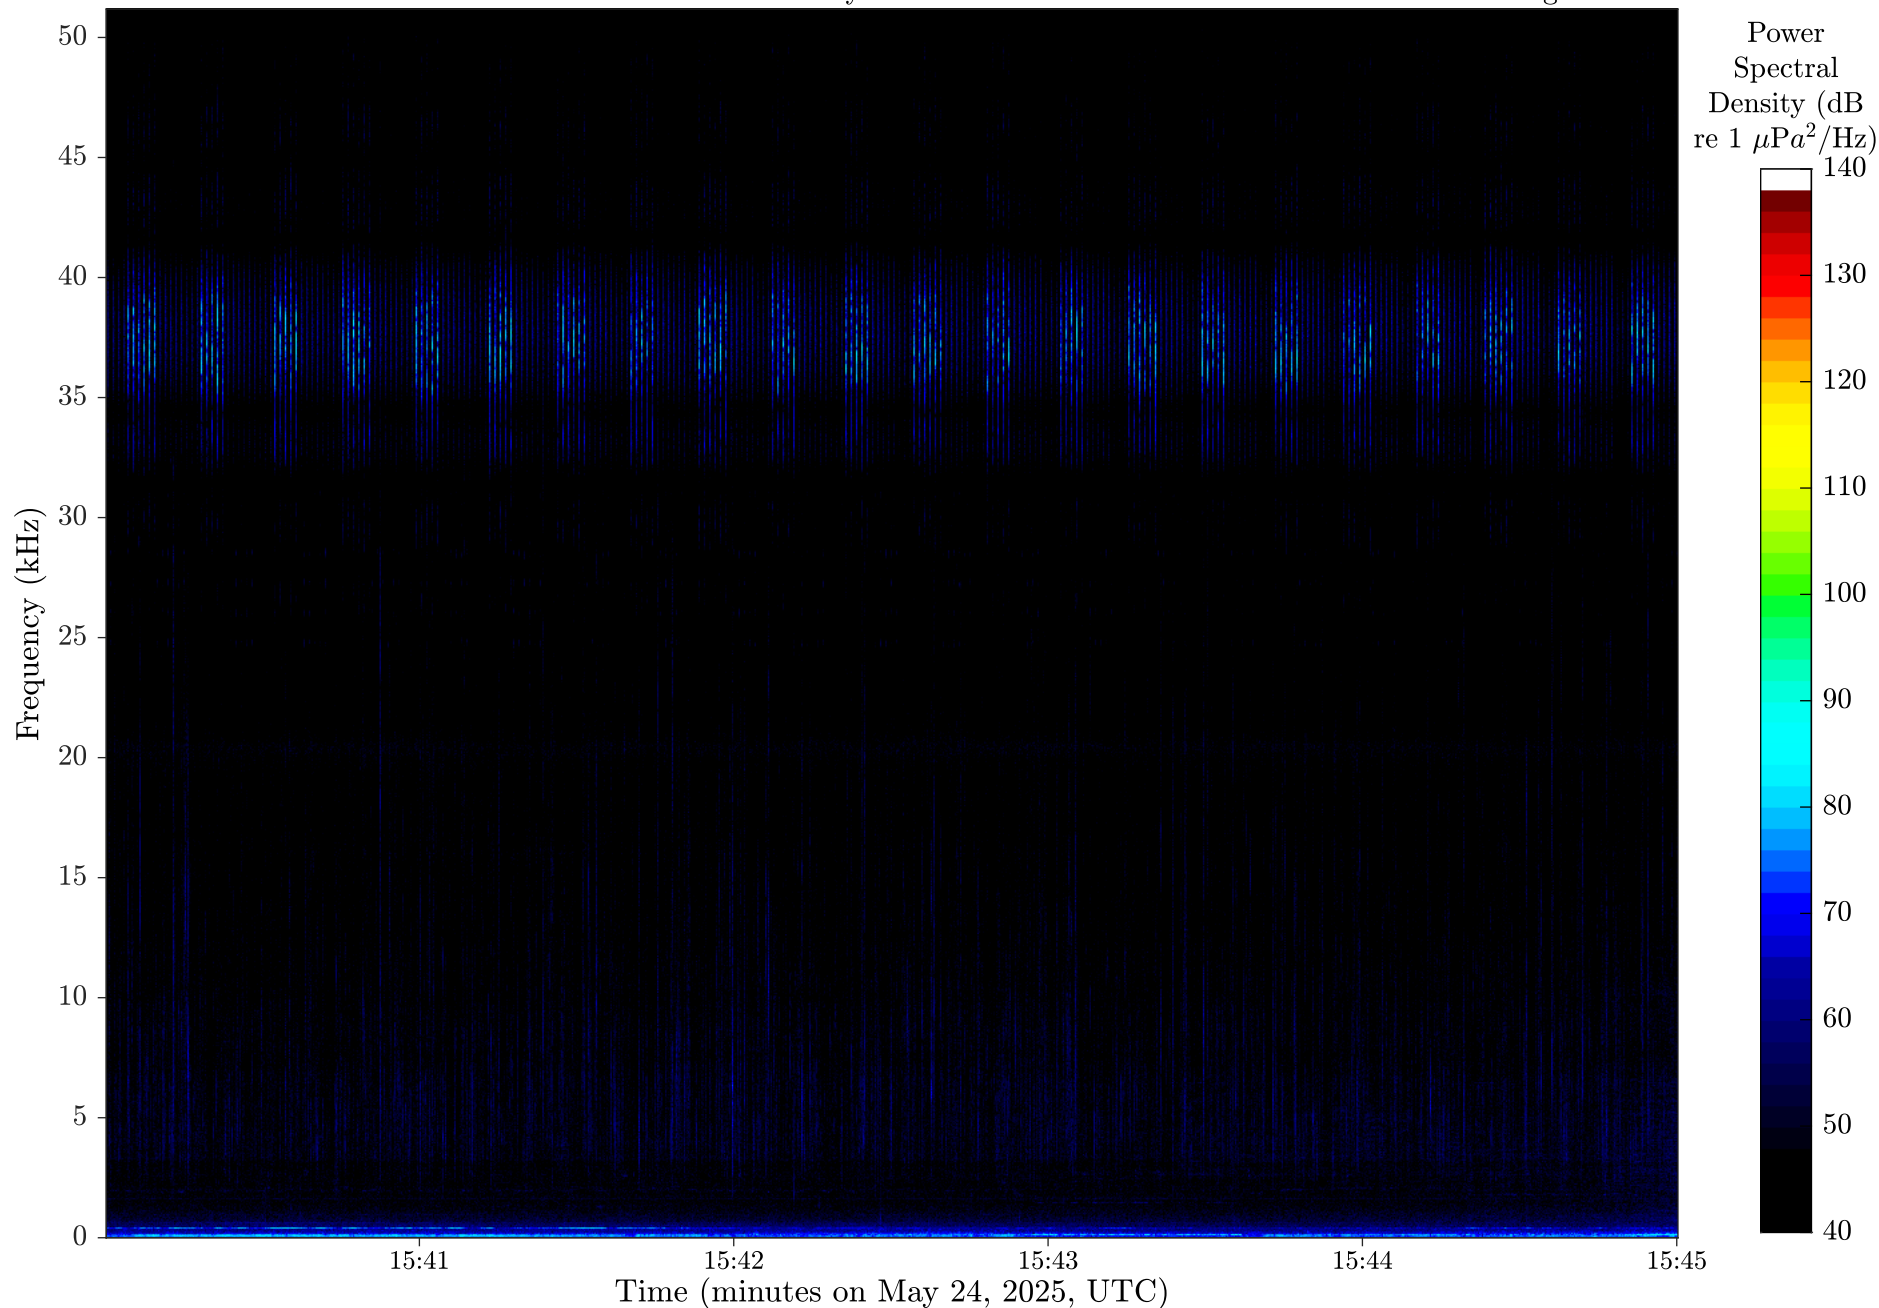

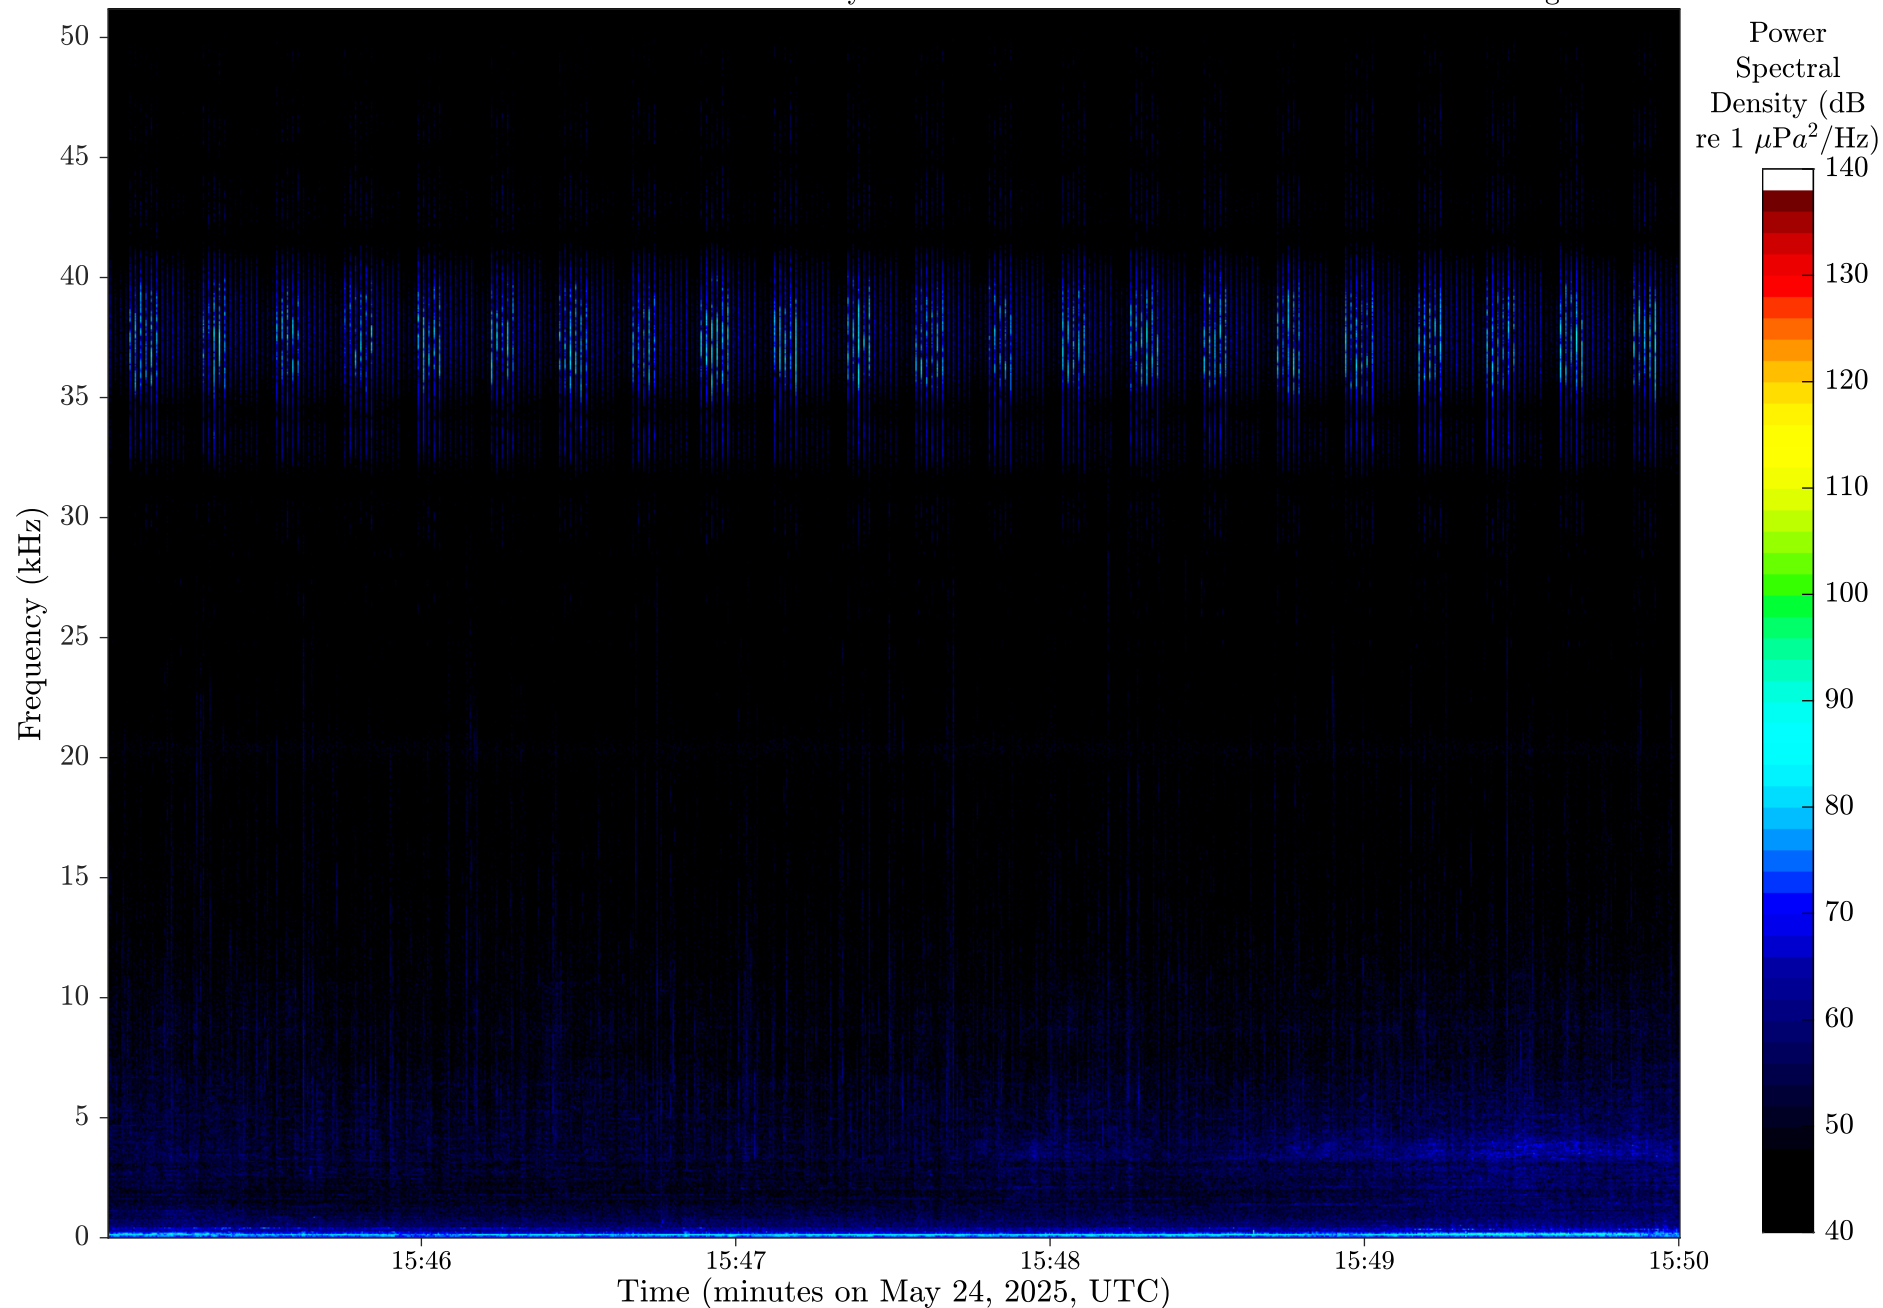


Comments: 32.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:44 UTC

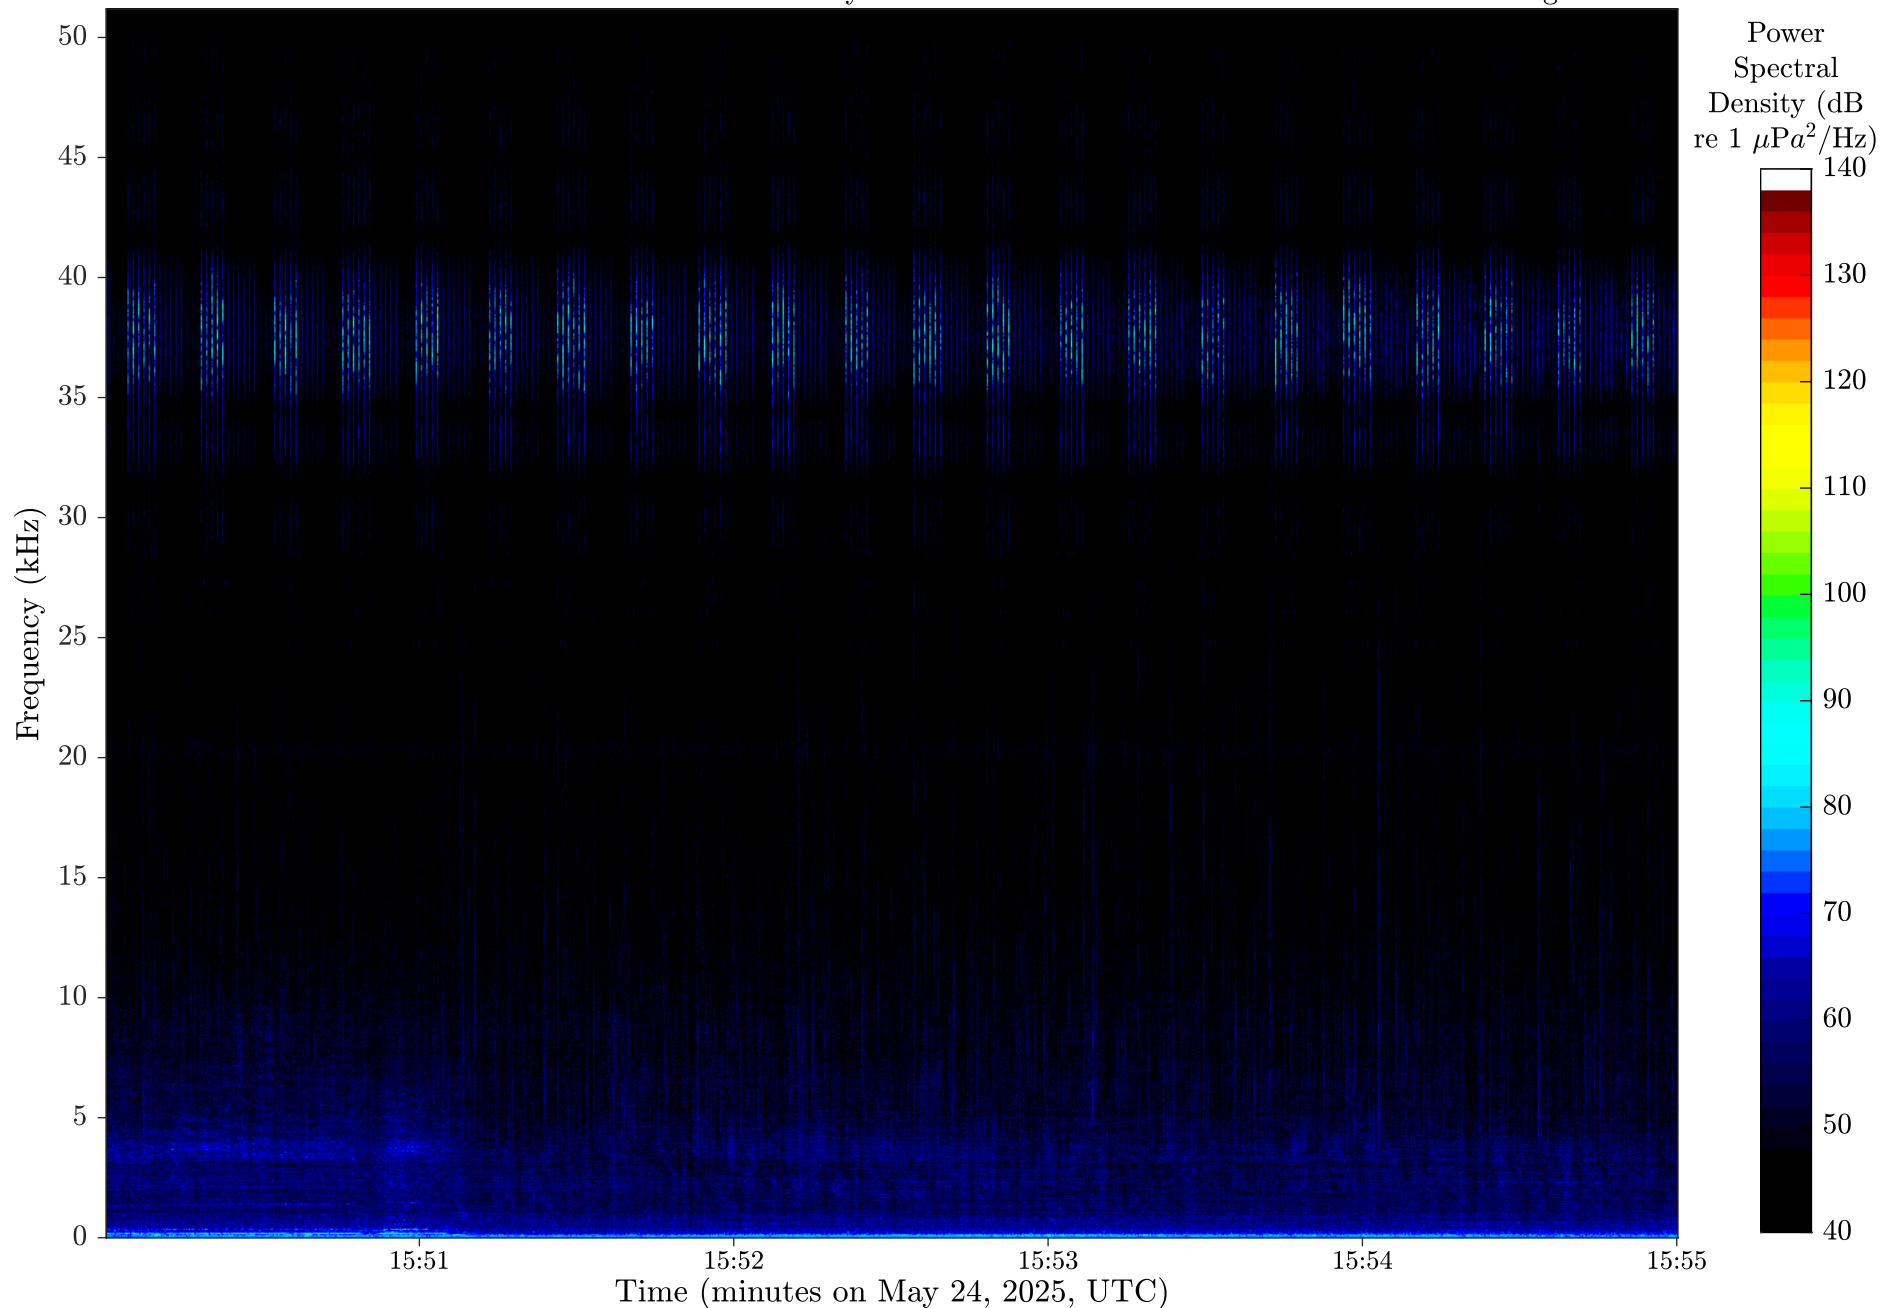


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:44:52 UTC

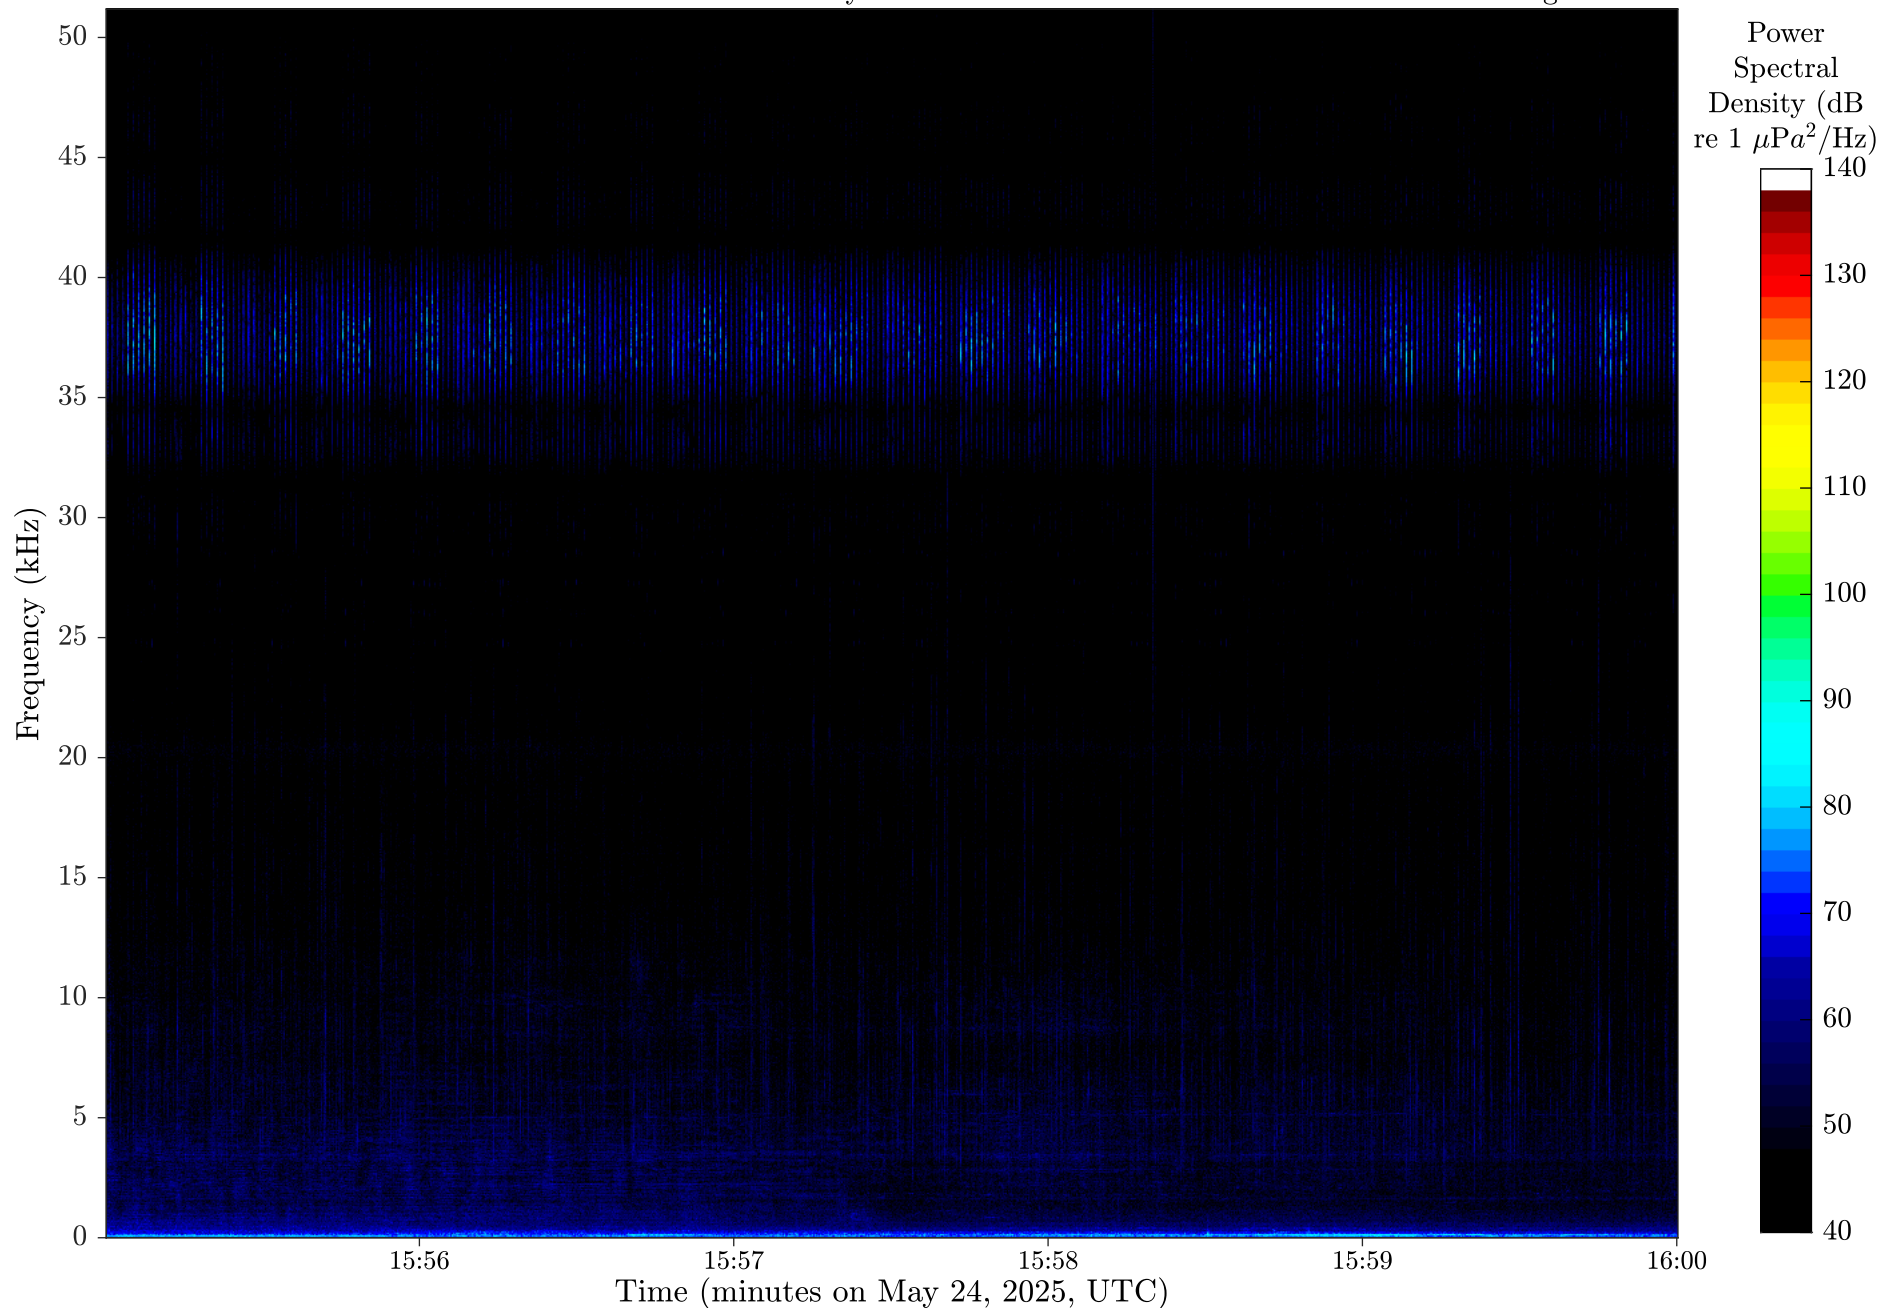


Comments: 31 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:45:00 UTC

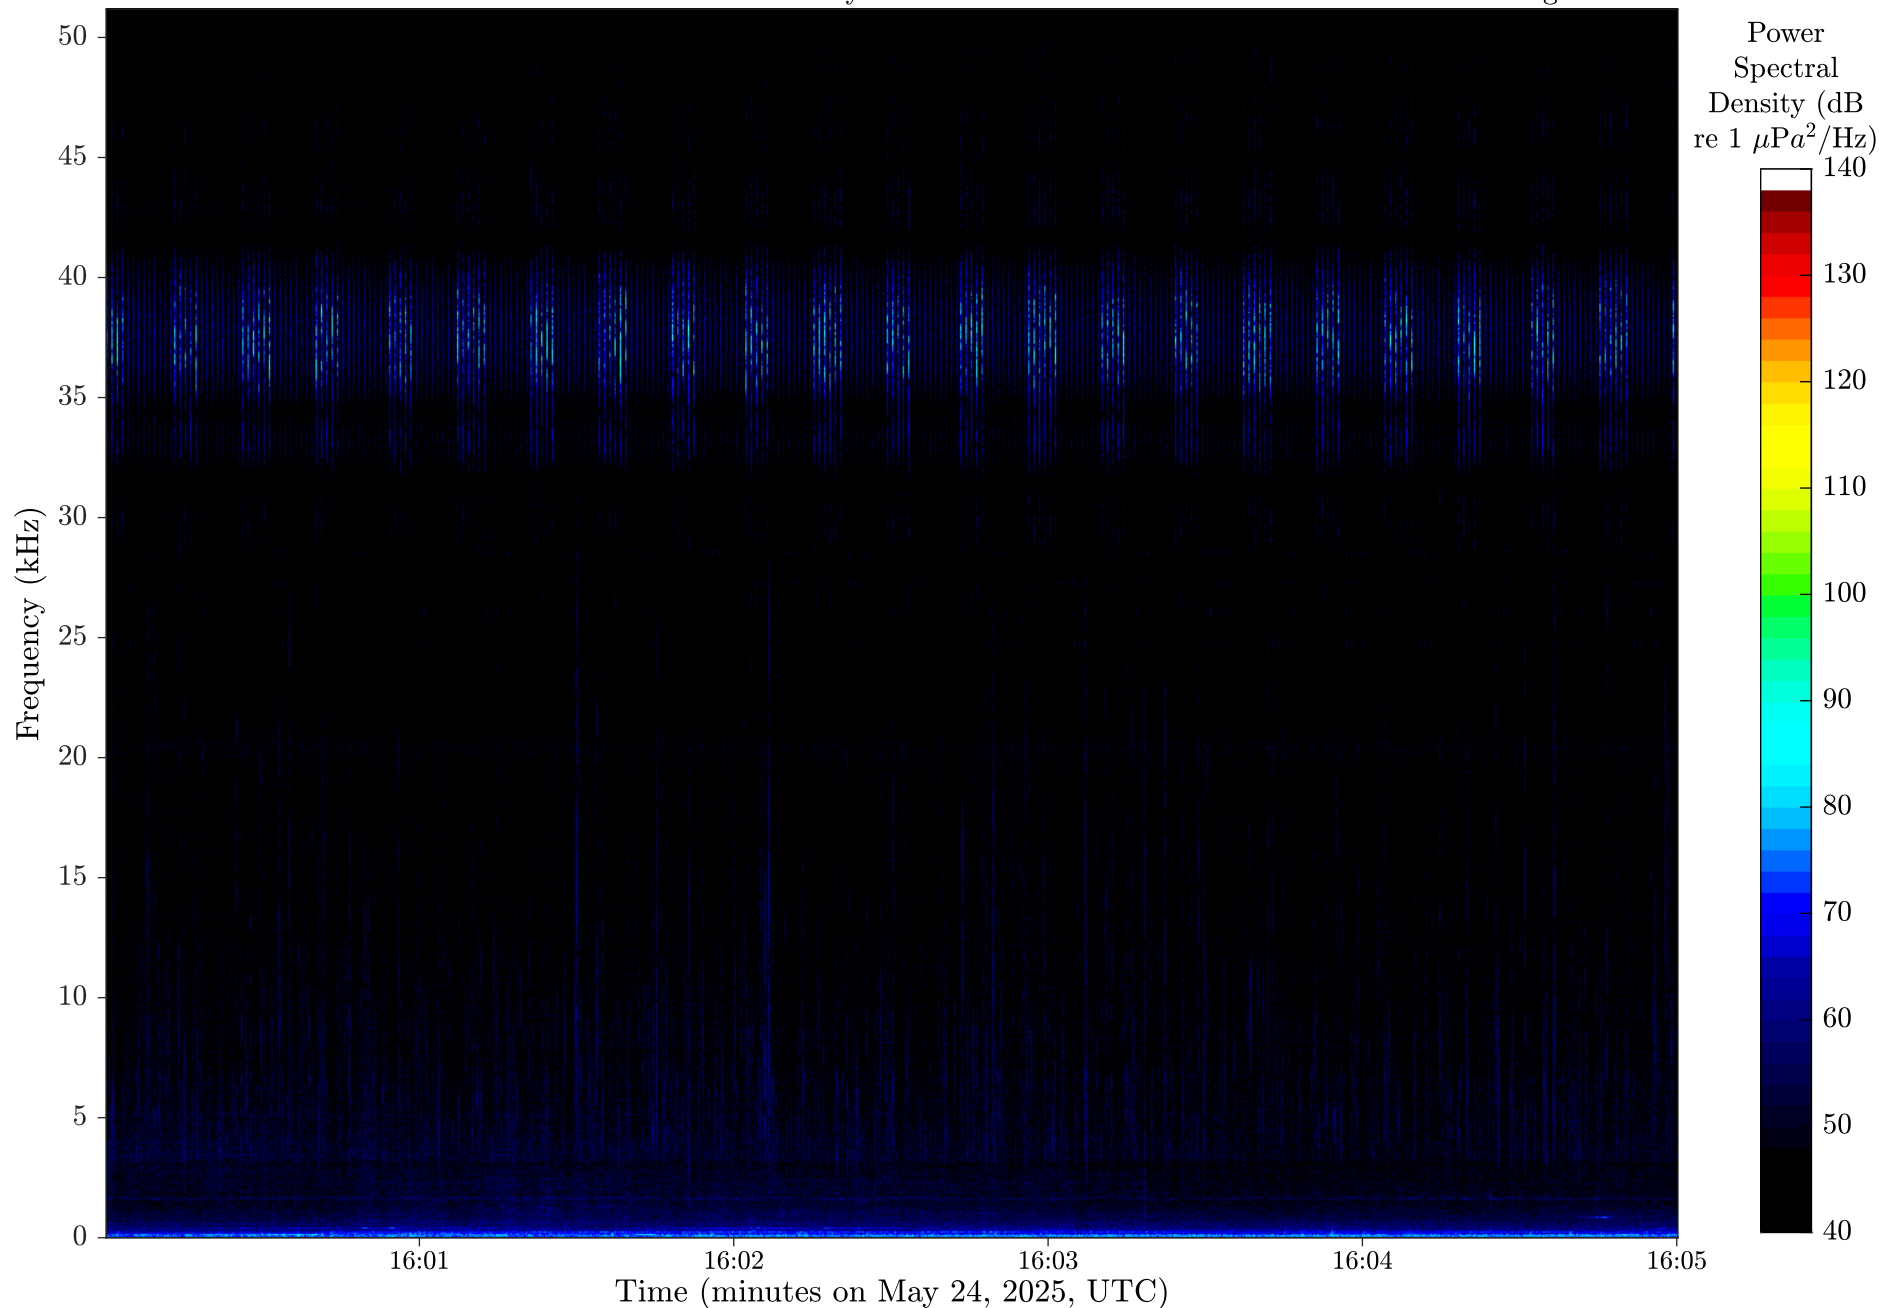


Comments: 31.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:45:08 UTC

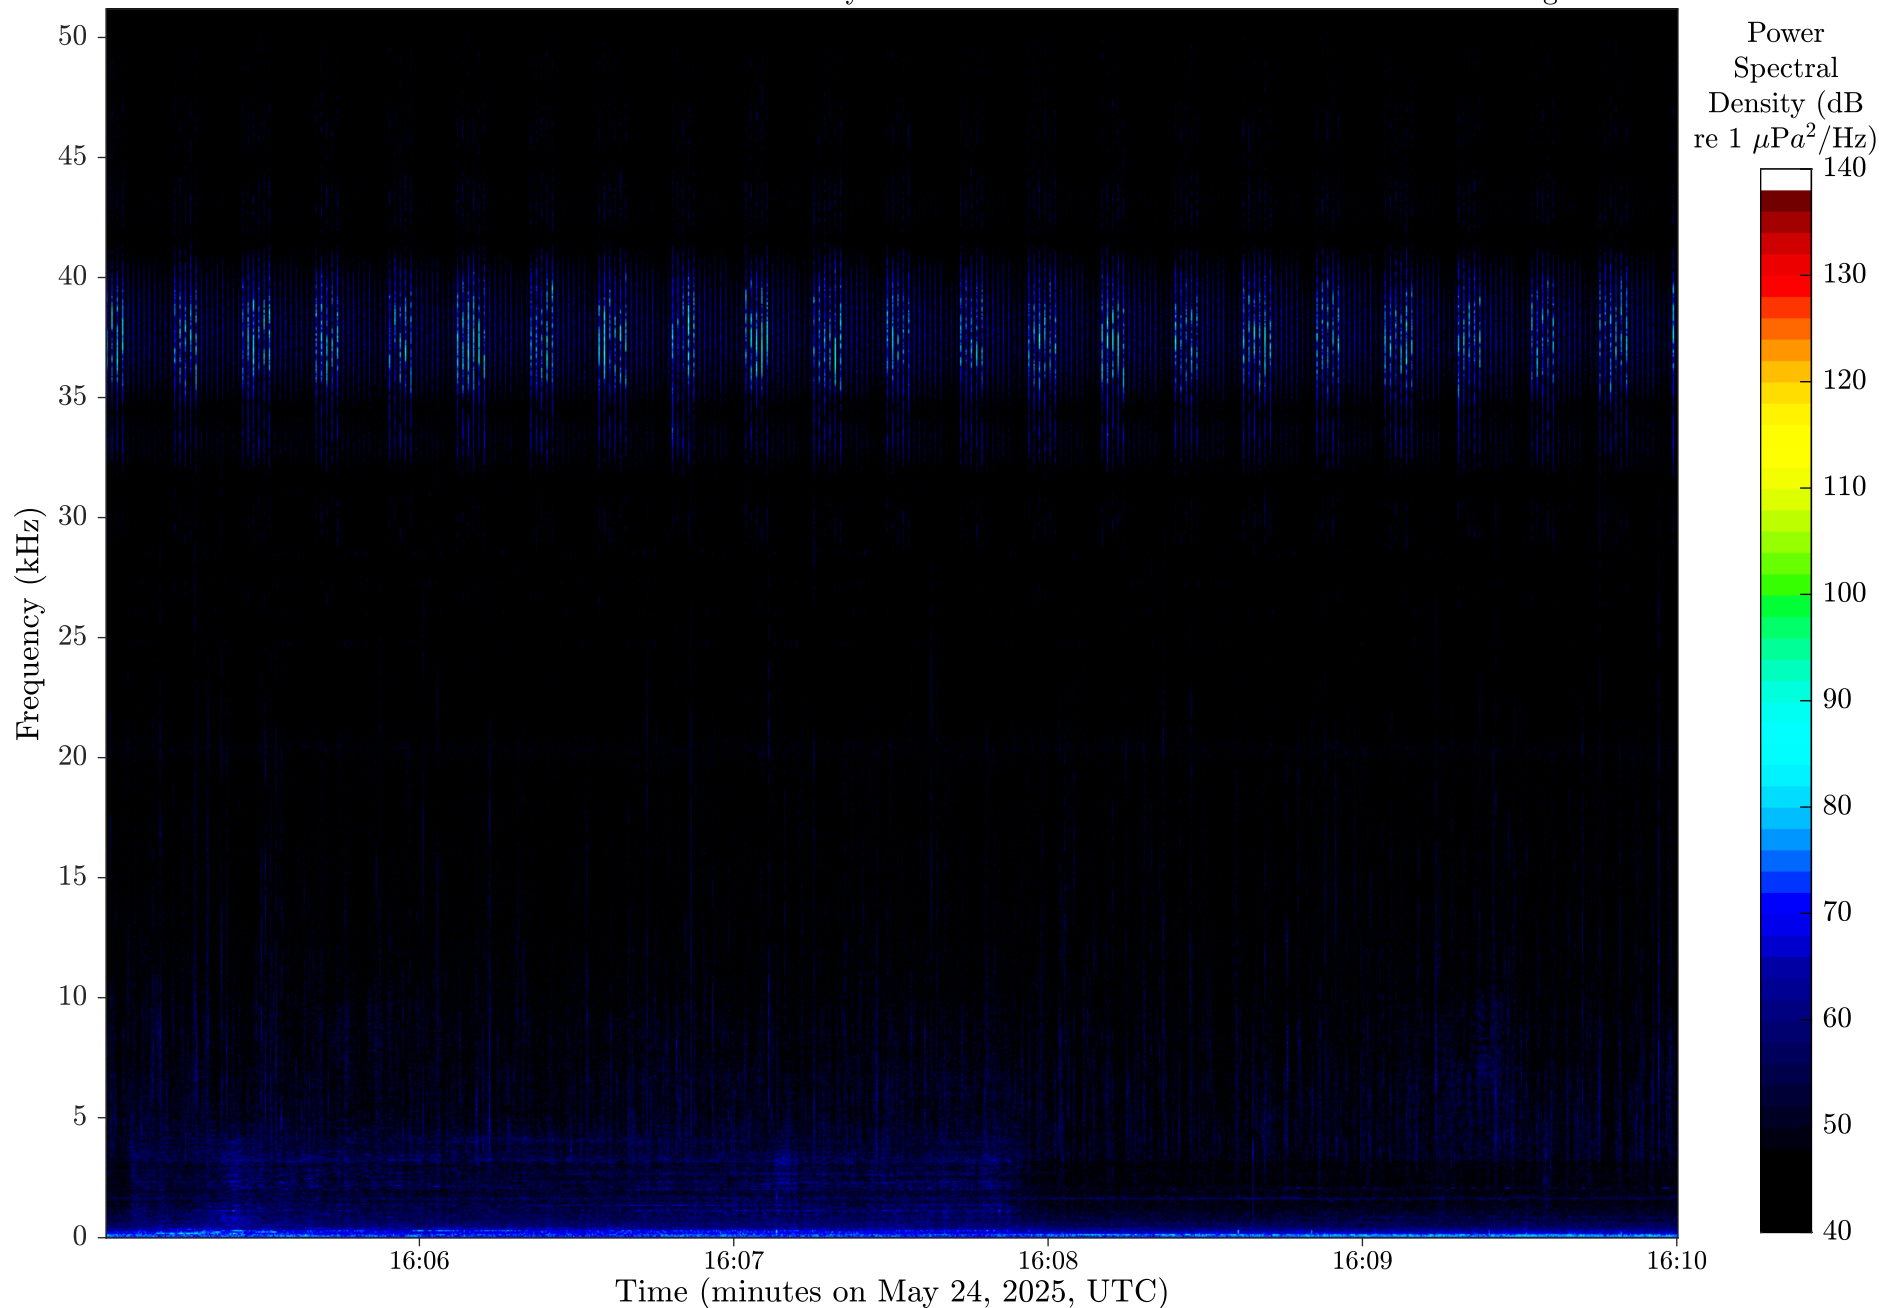


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:45:16 UTC

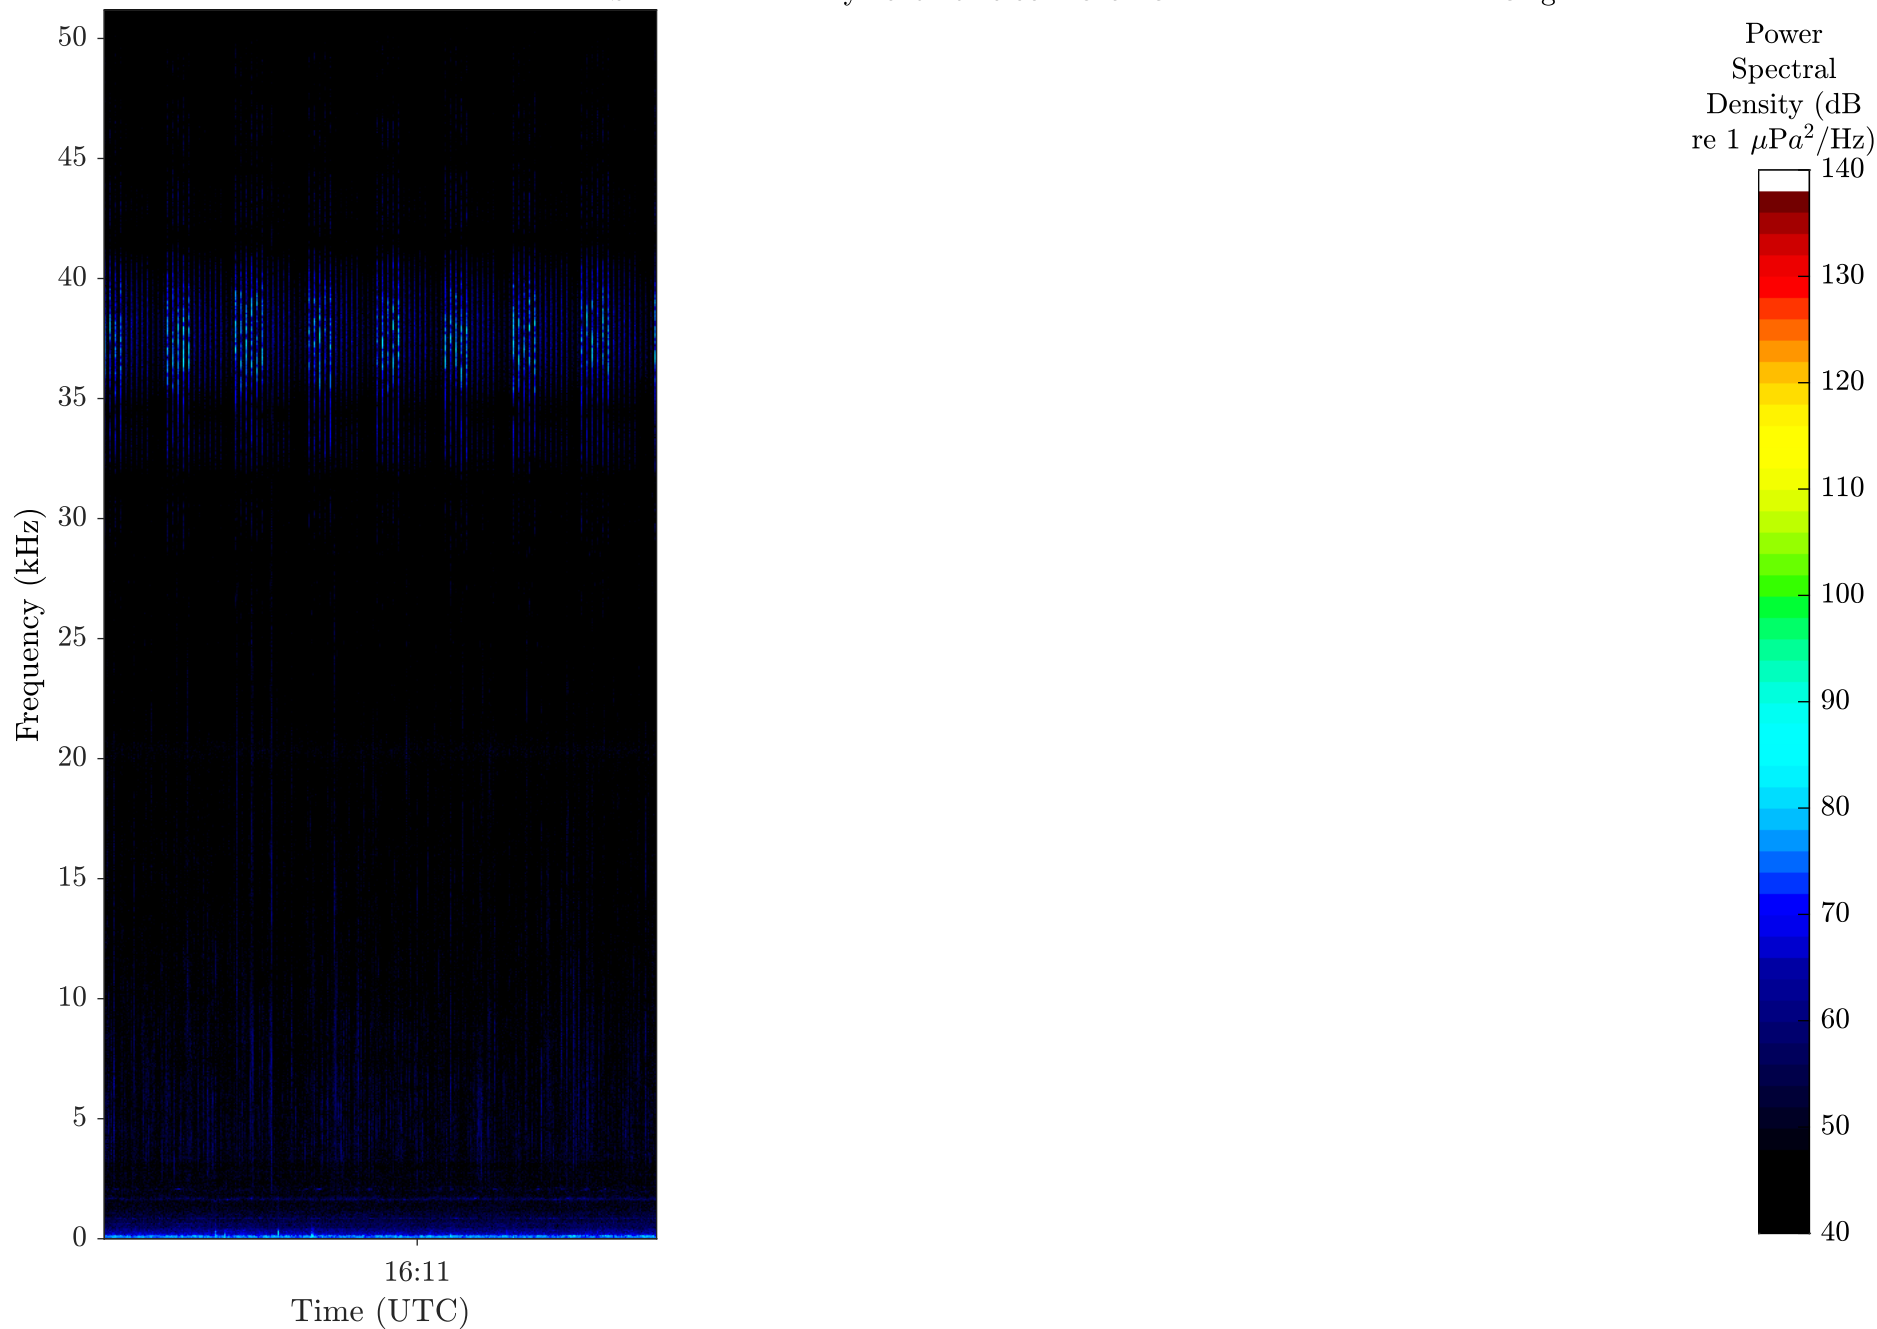

Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:45:20 UTC

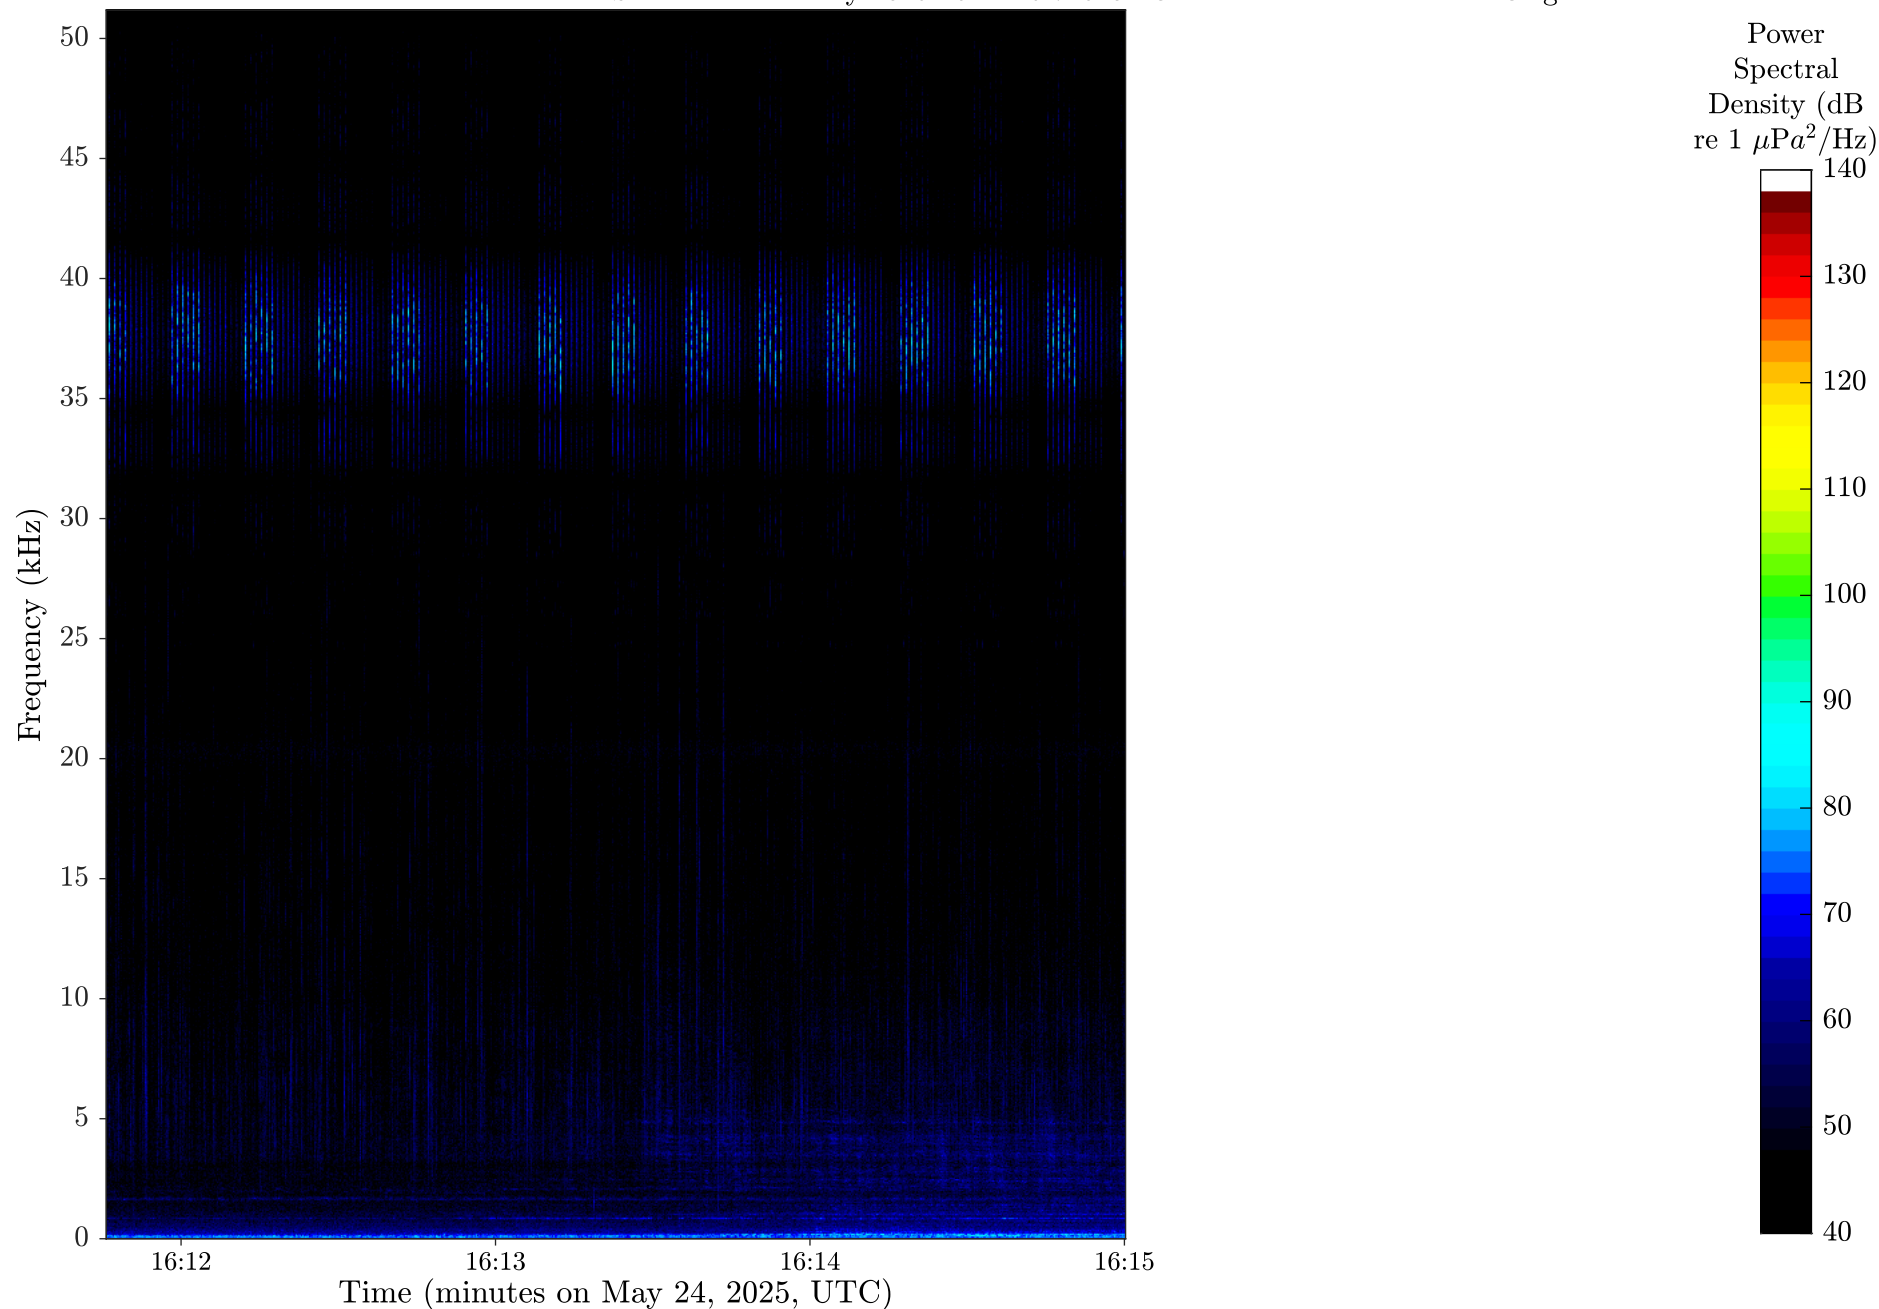

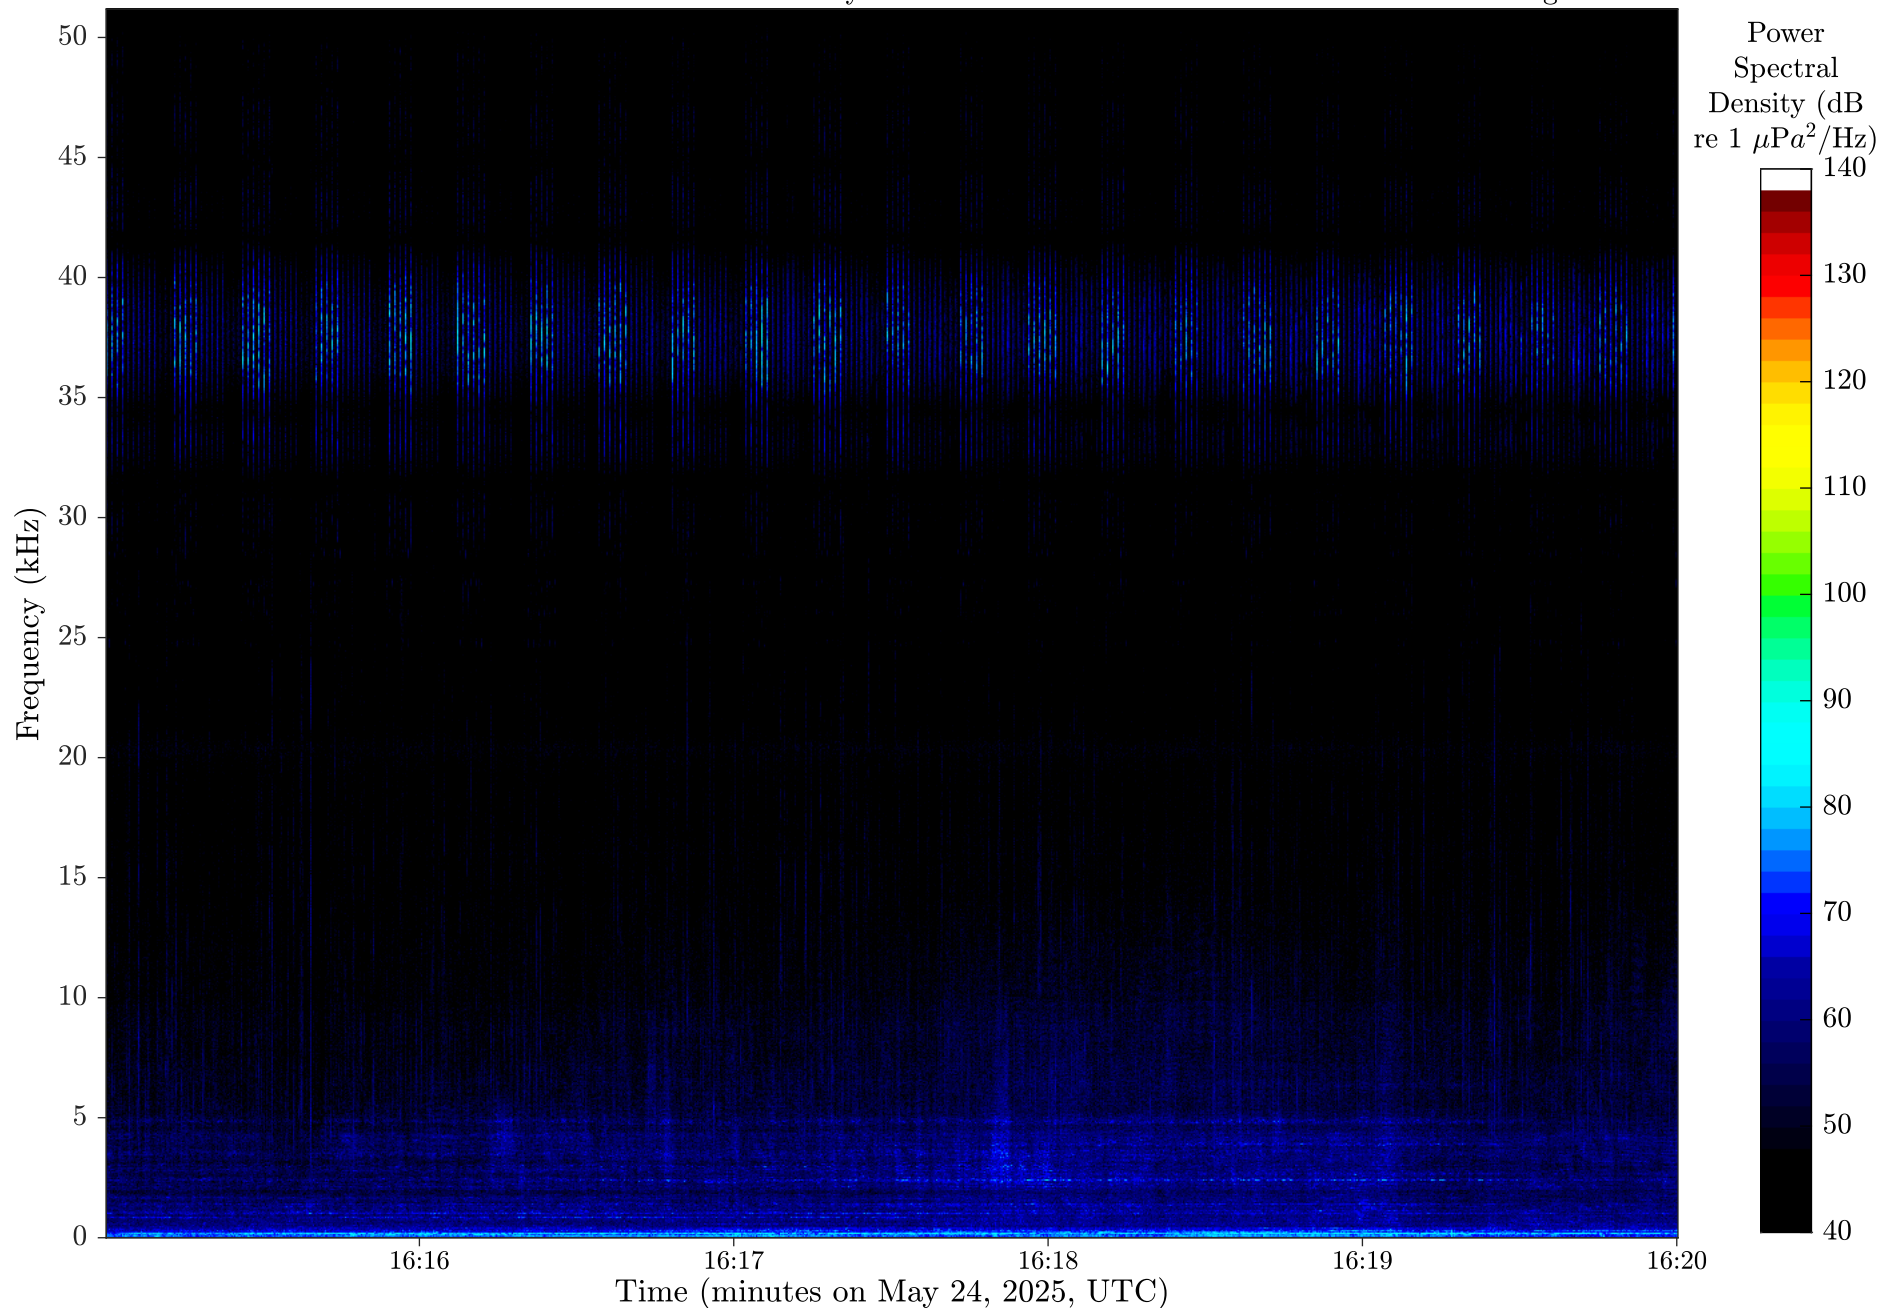


Comments: 29.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:45:33 UTC

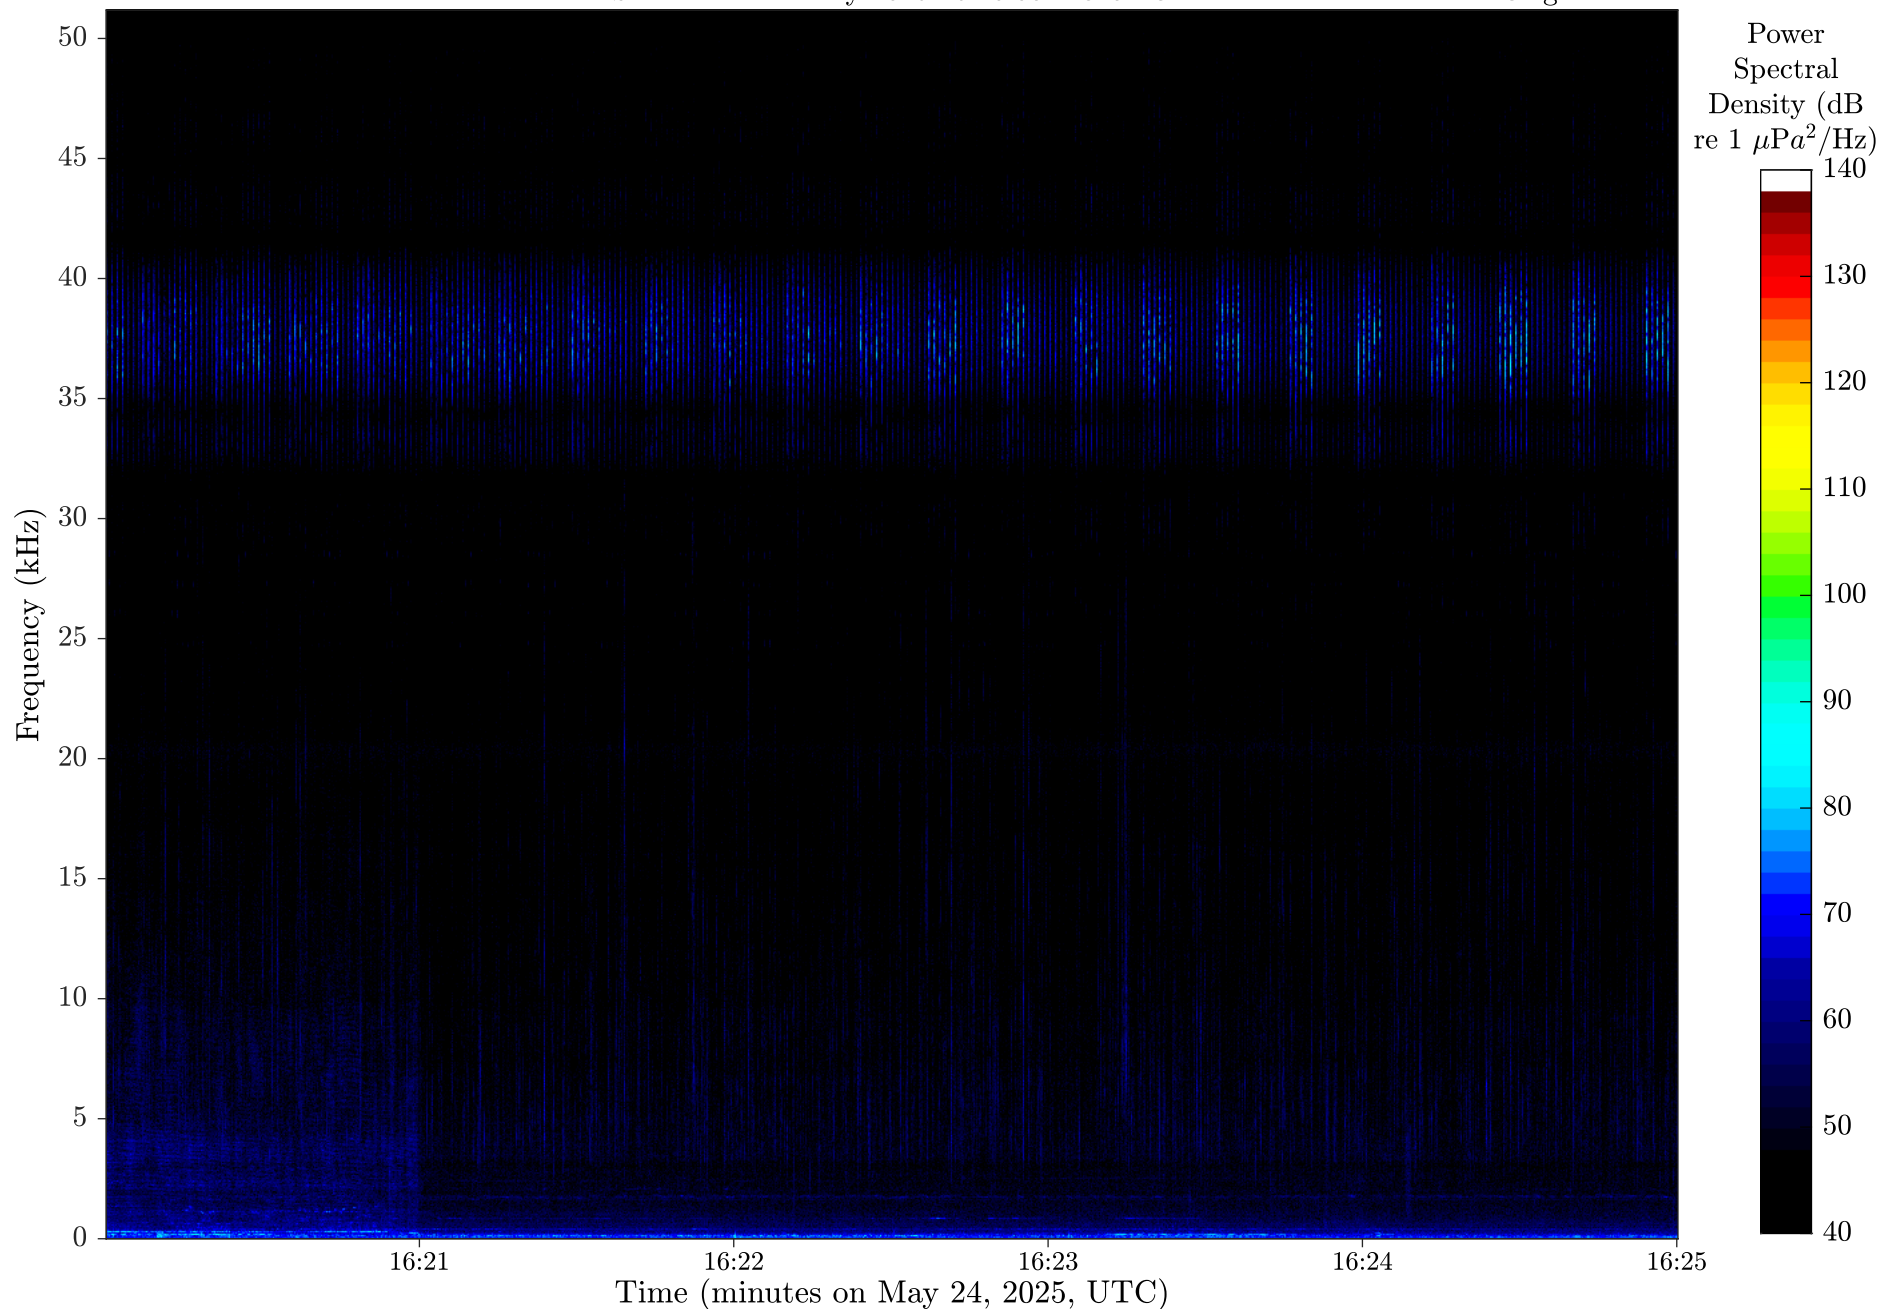

Comments: 29.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:45:41 UTC

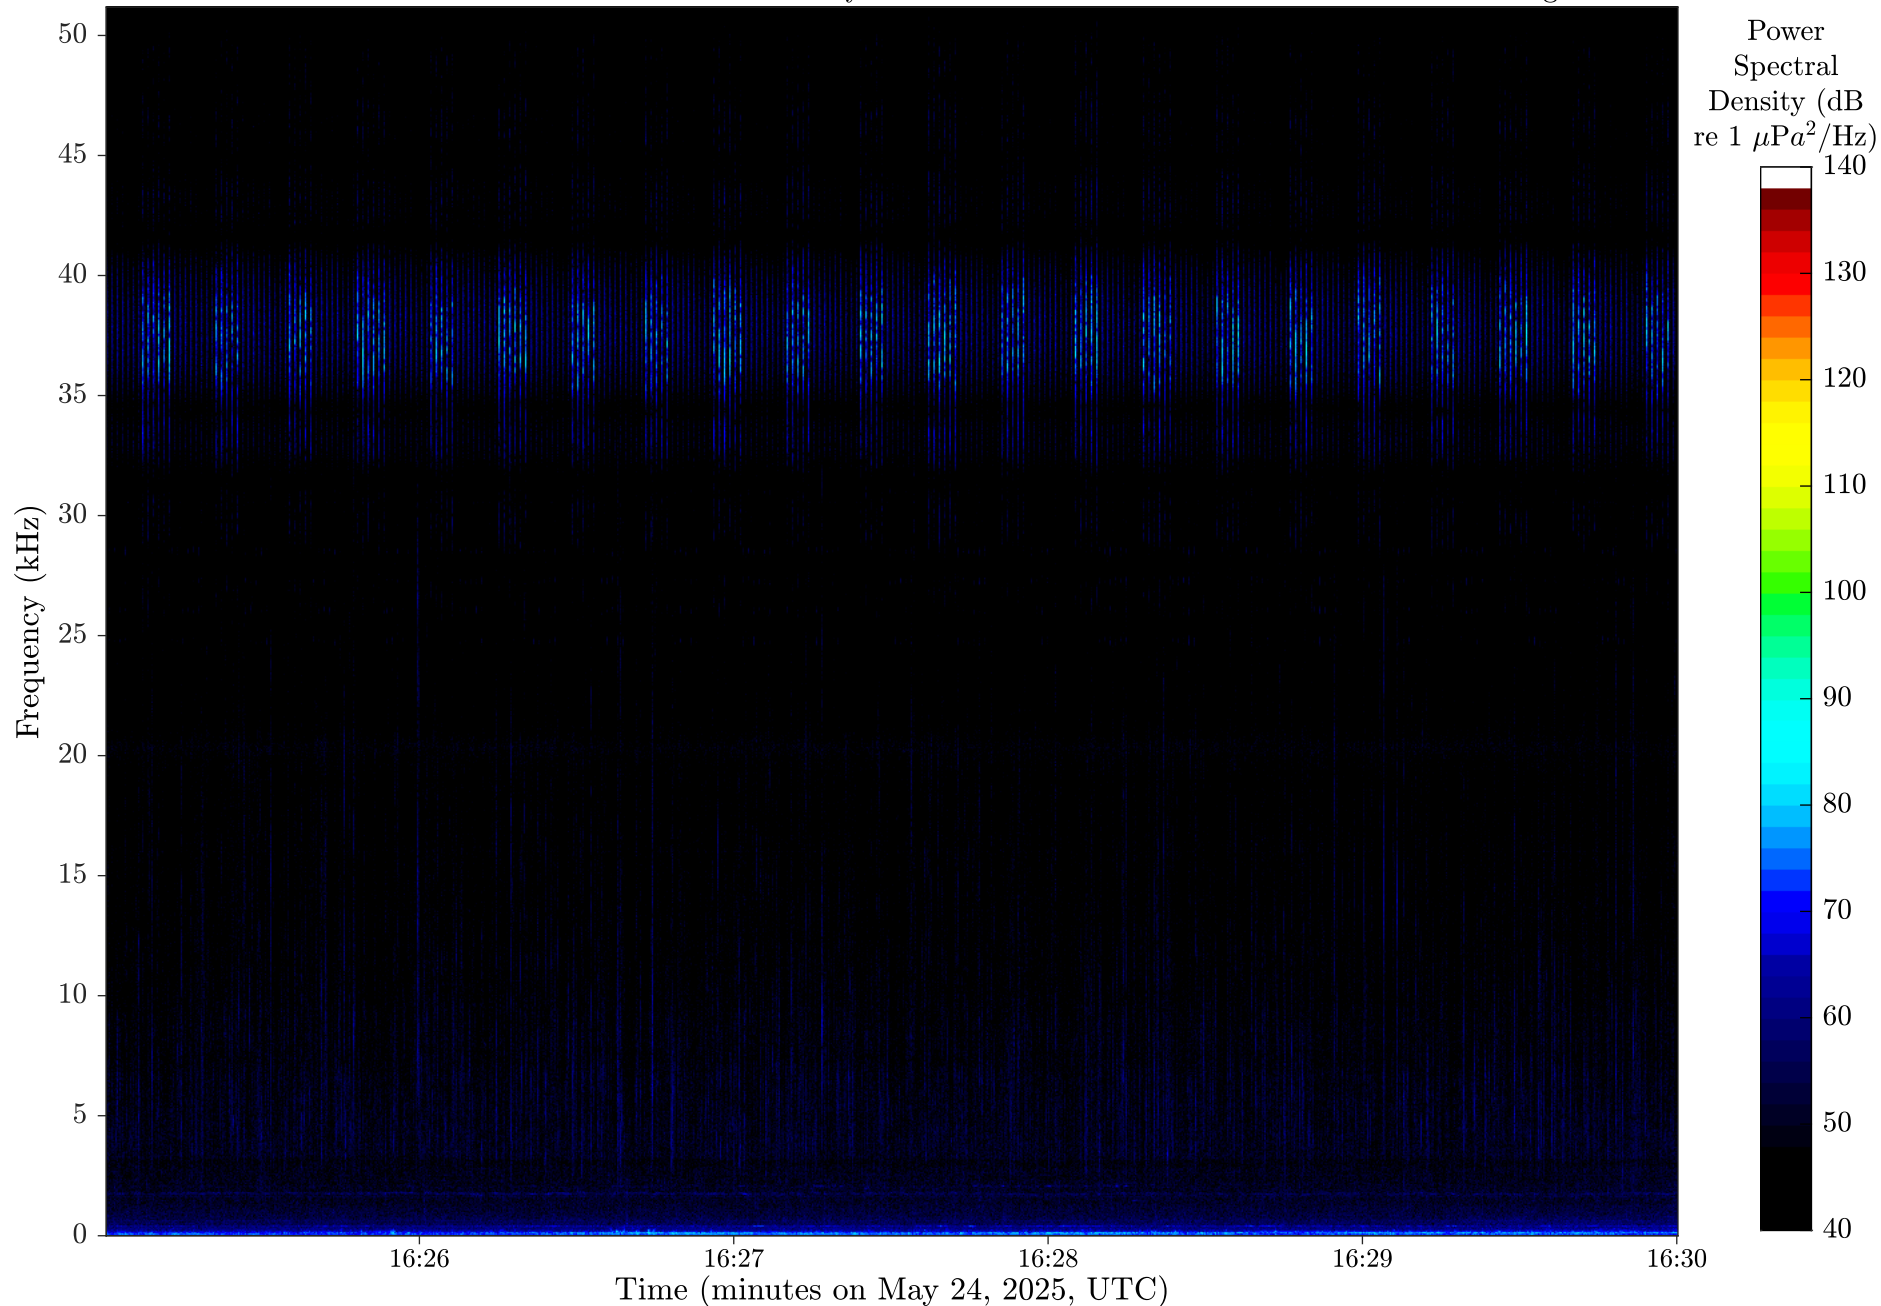

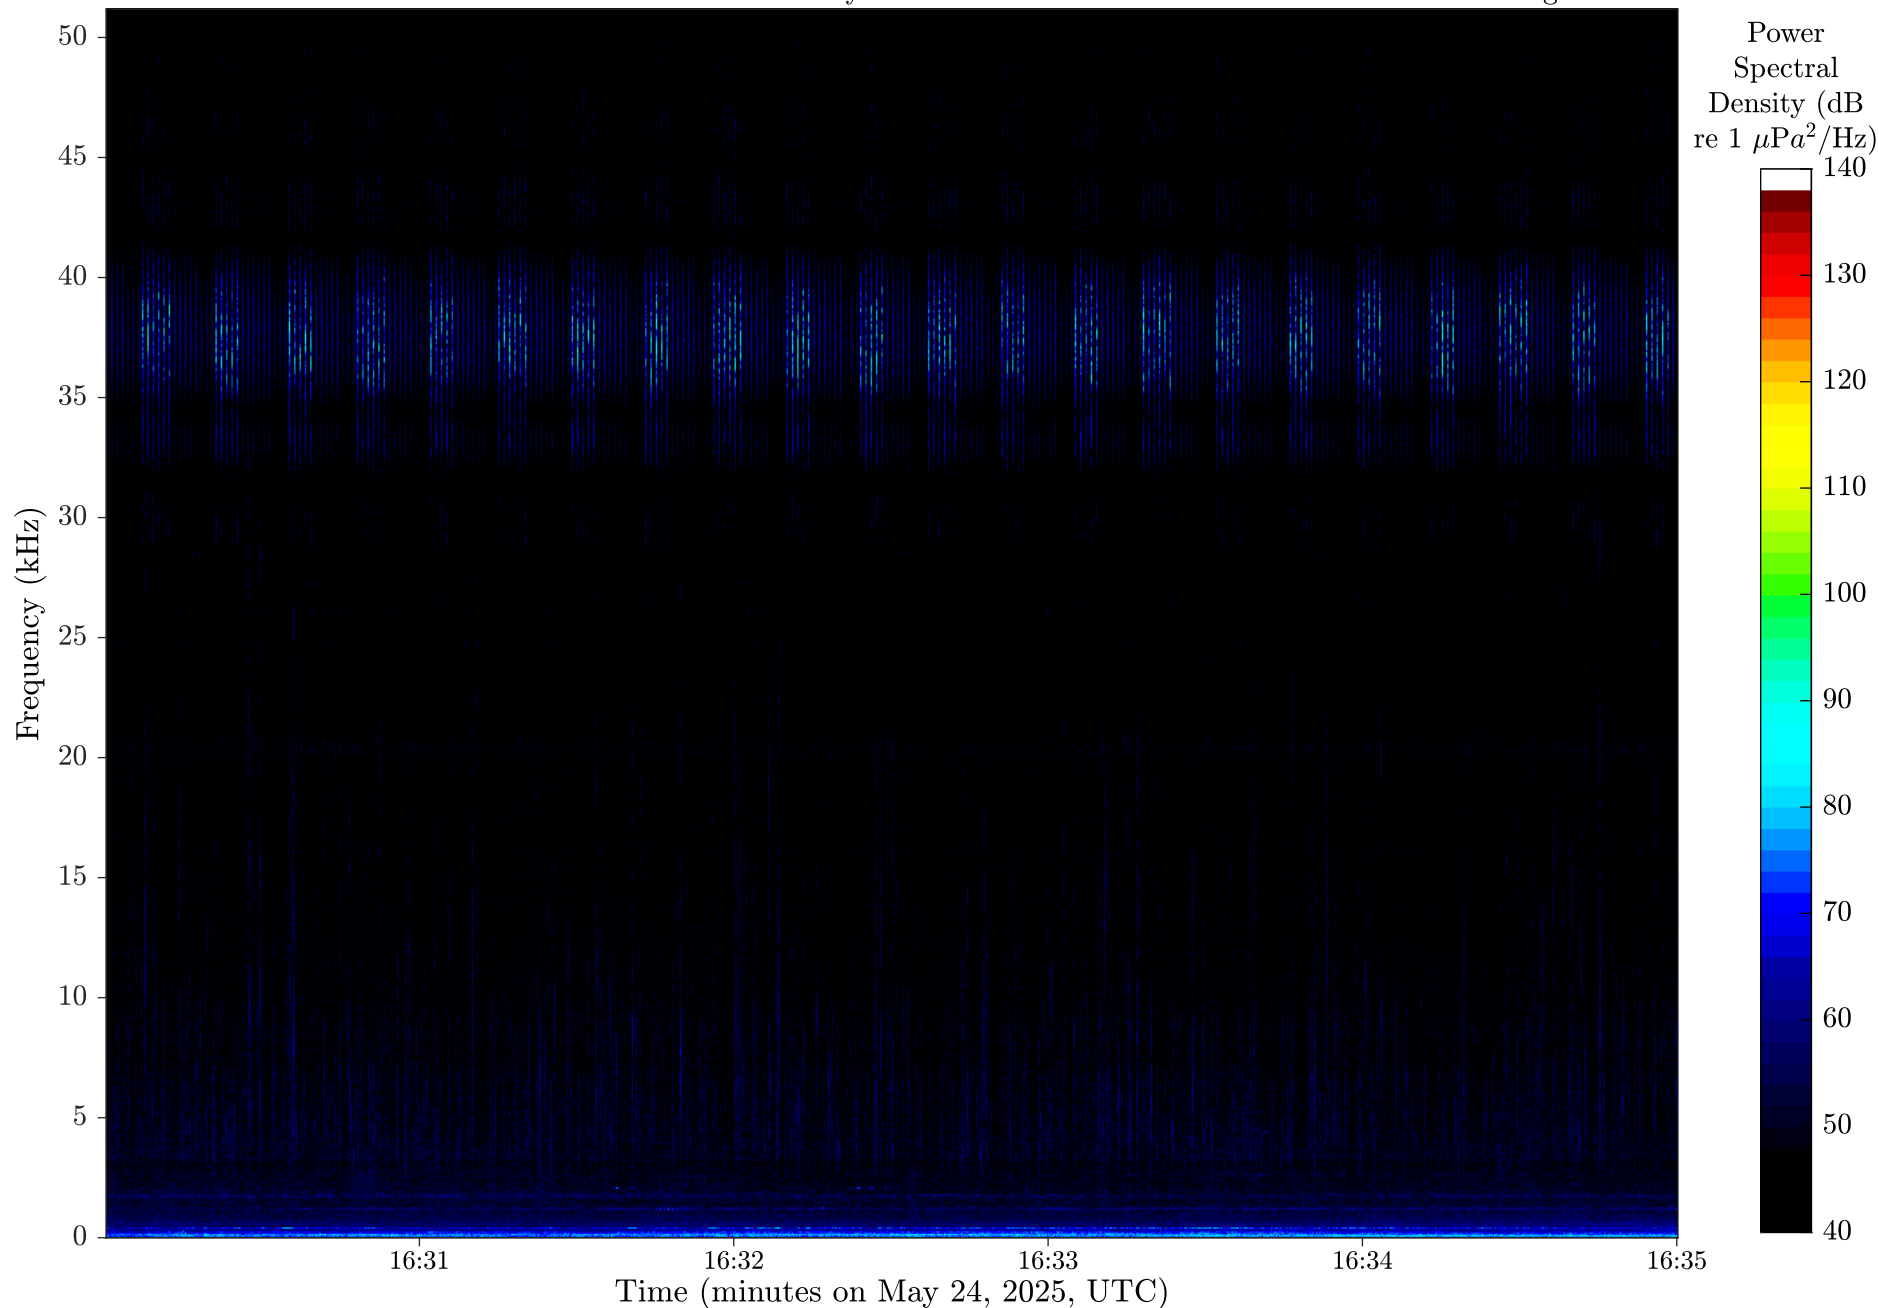


Comments: 31.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:45:56 UTC

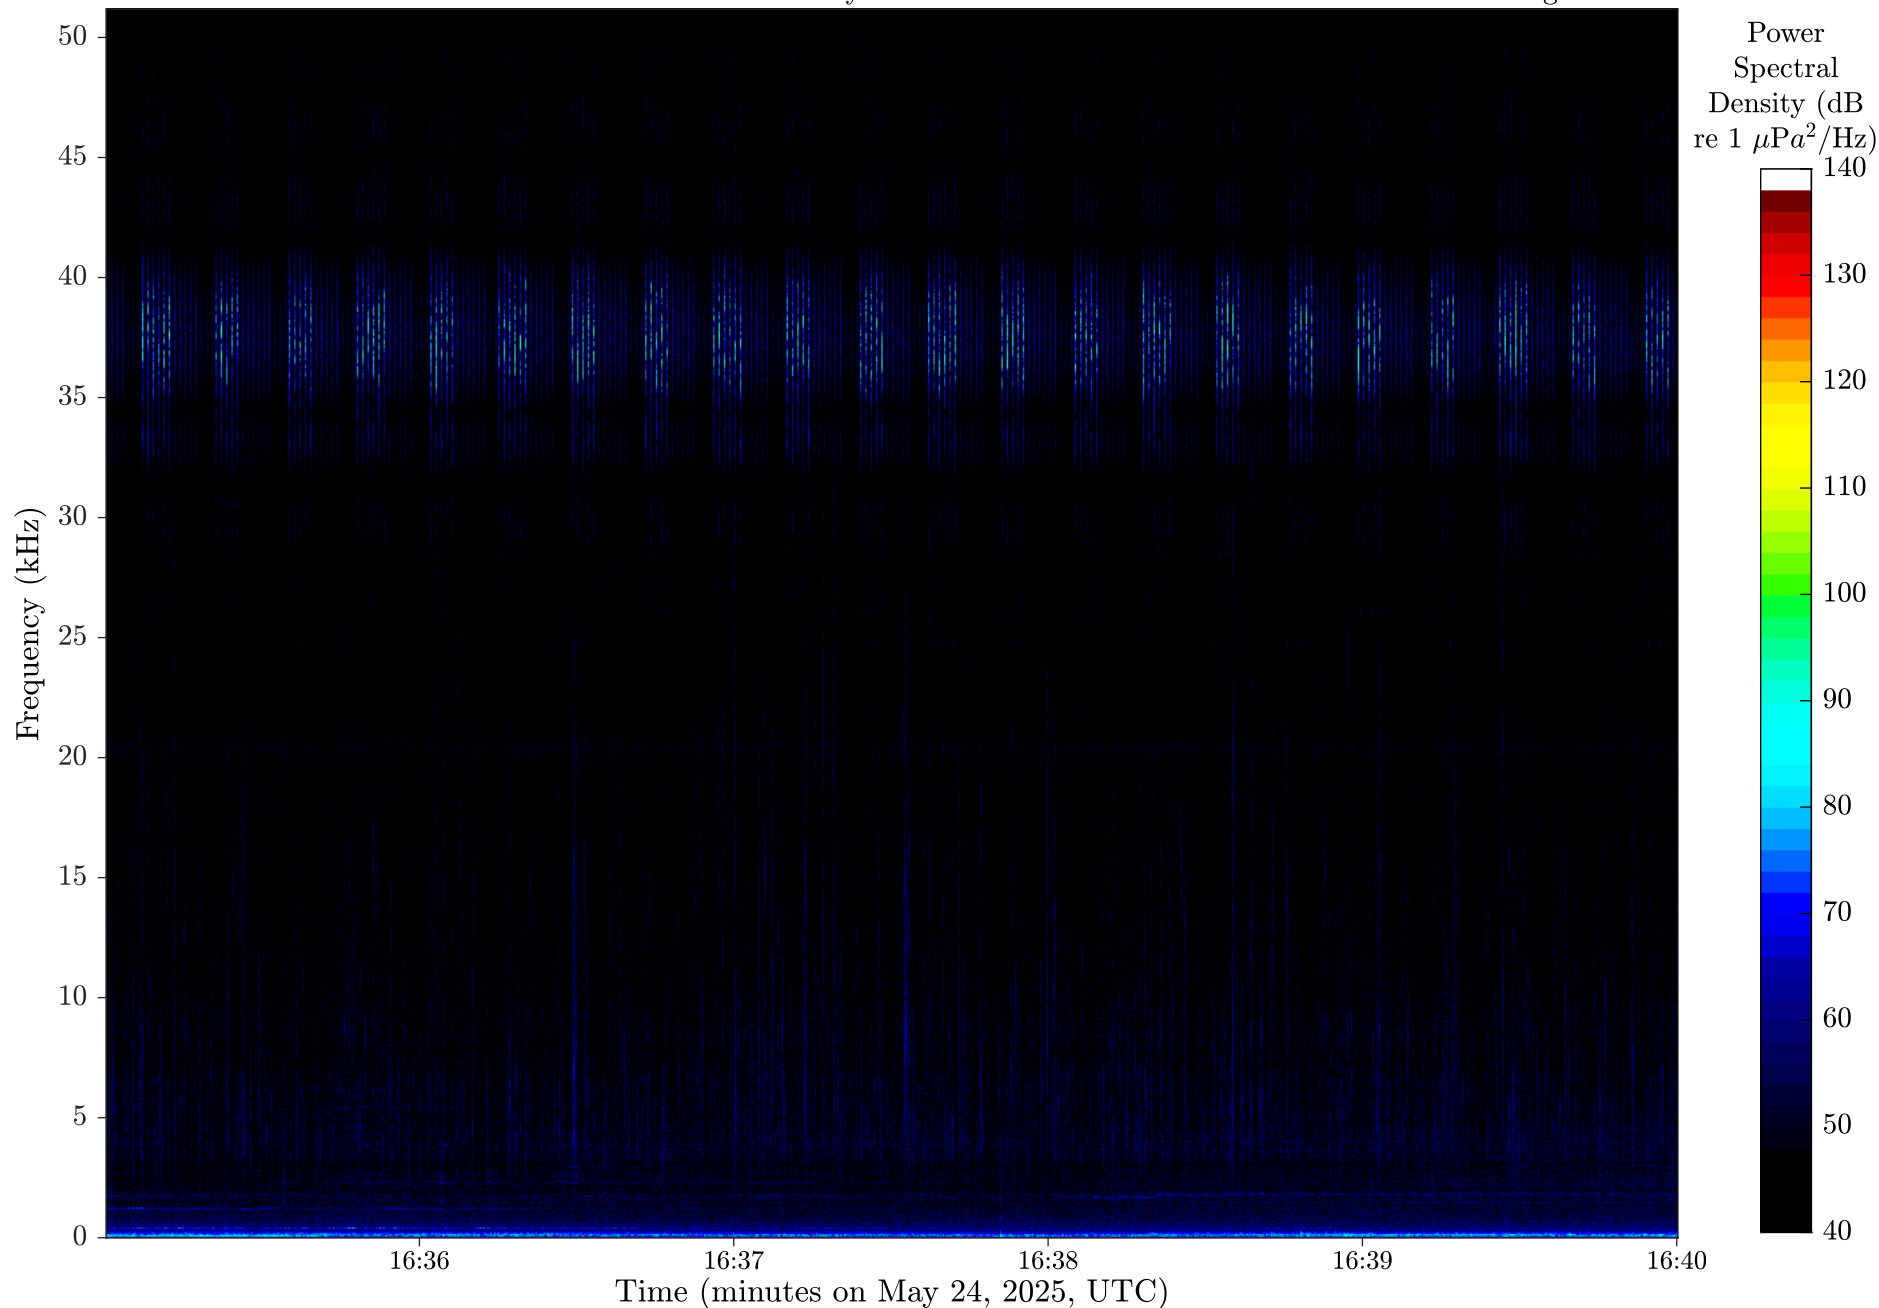



Comments: 30.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:04 UTC

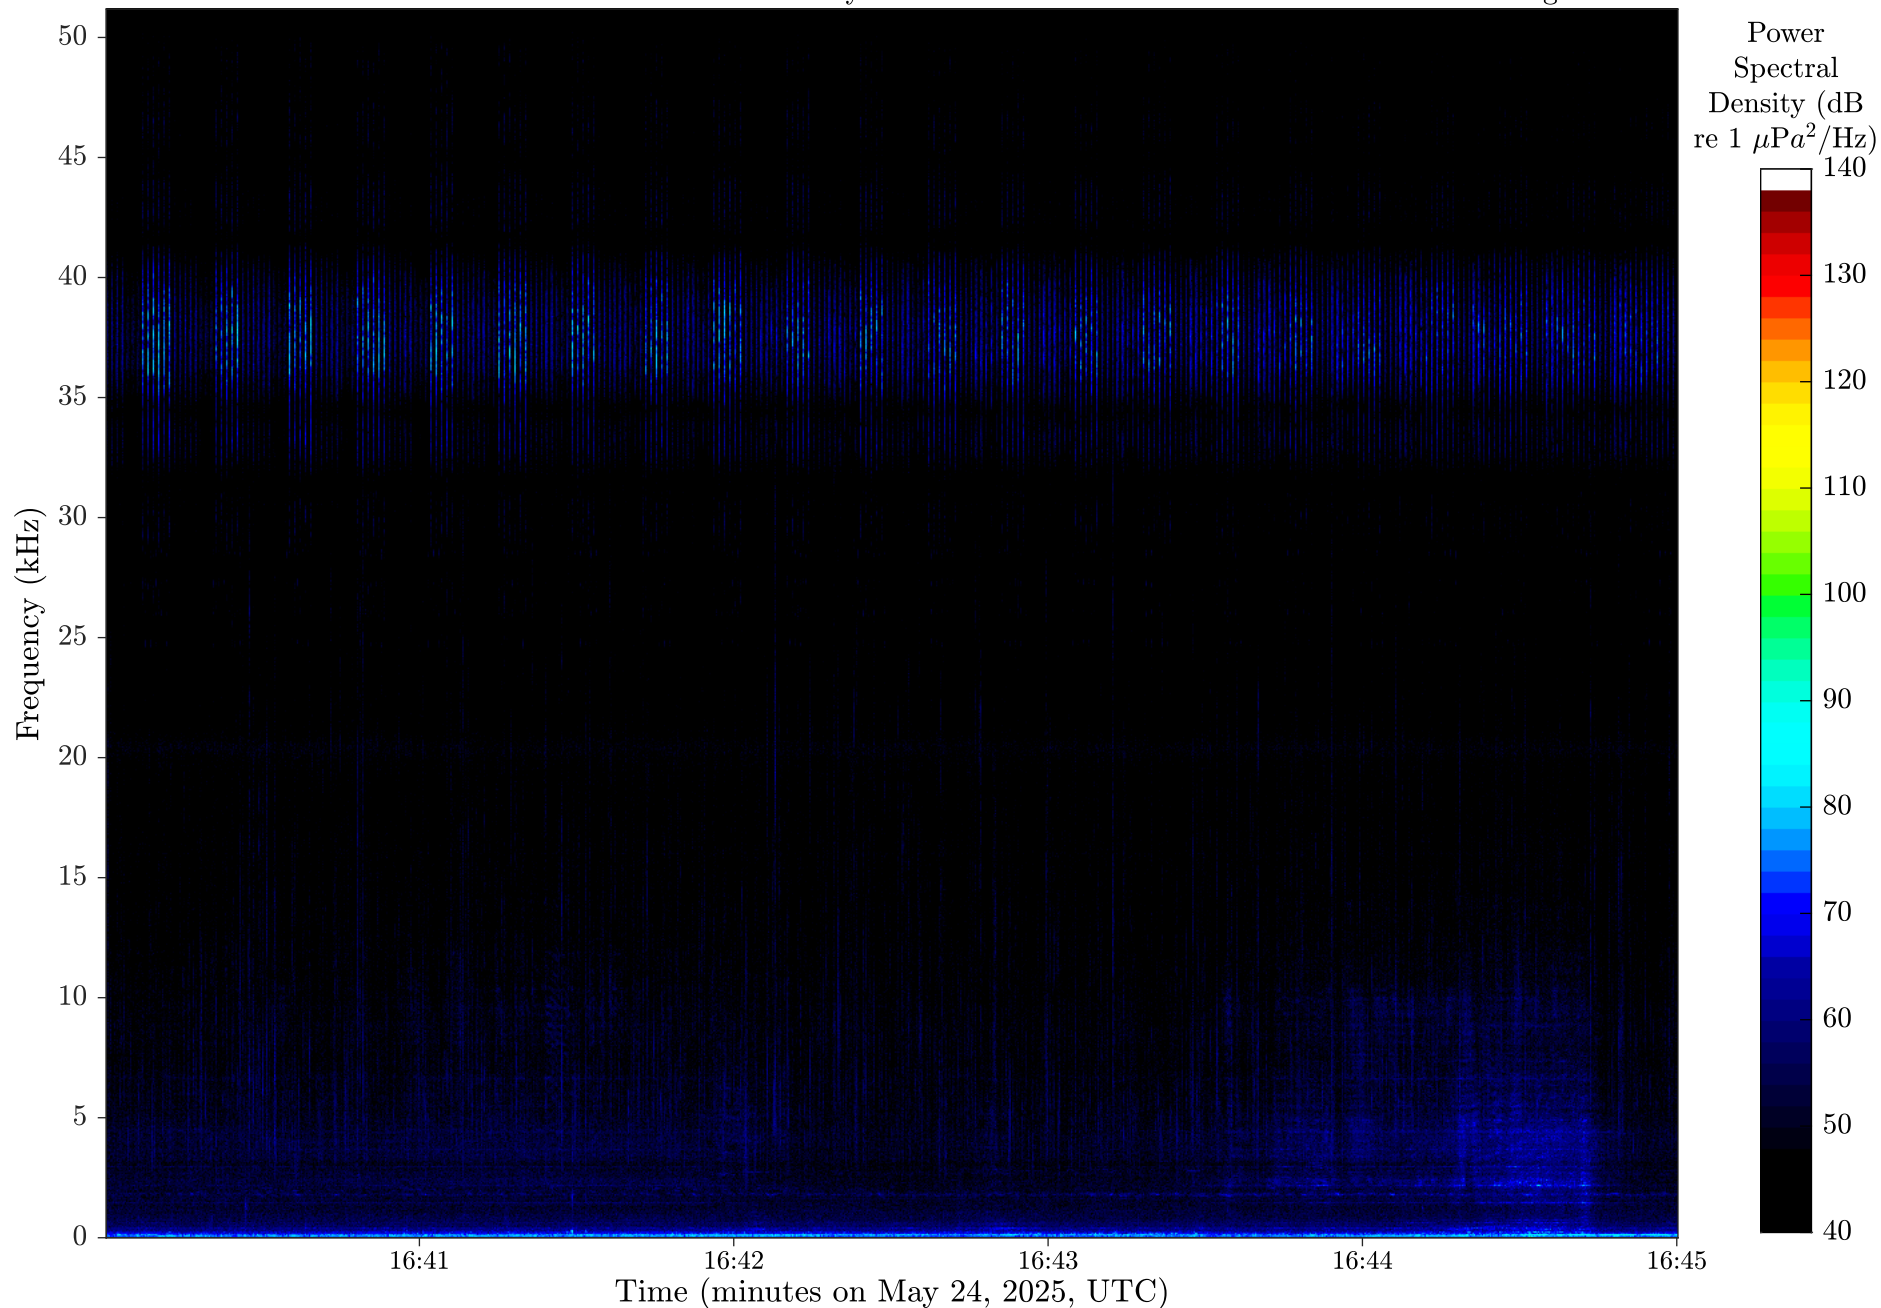

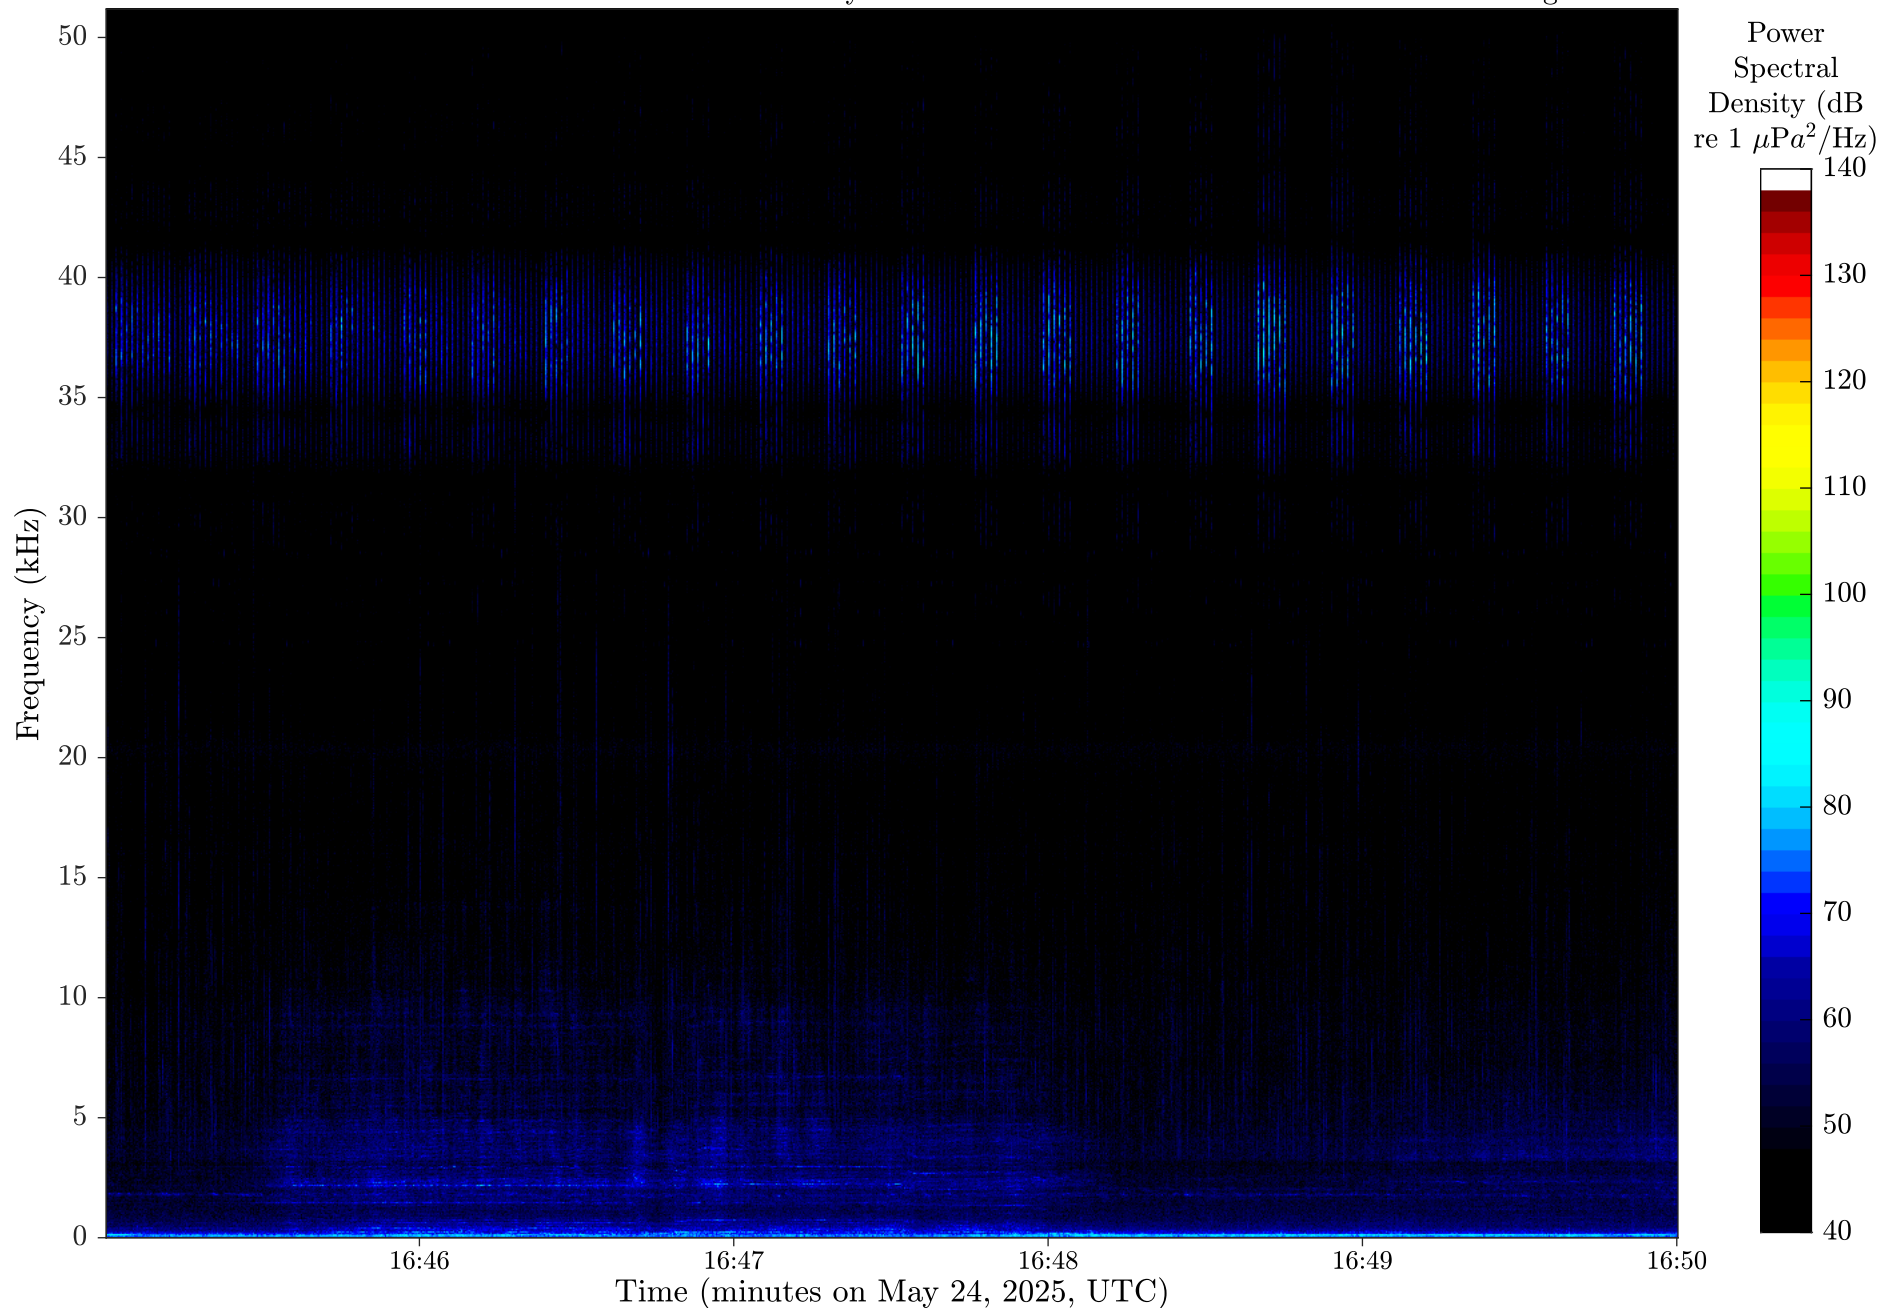


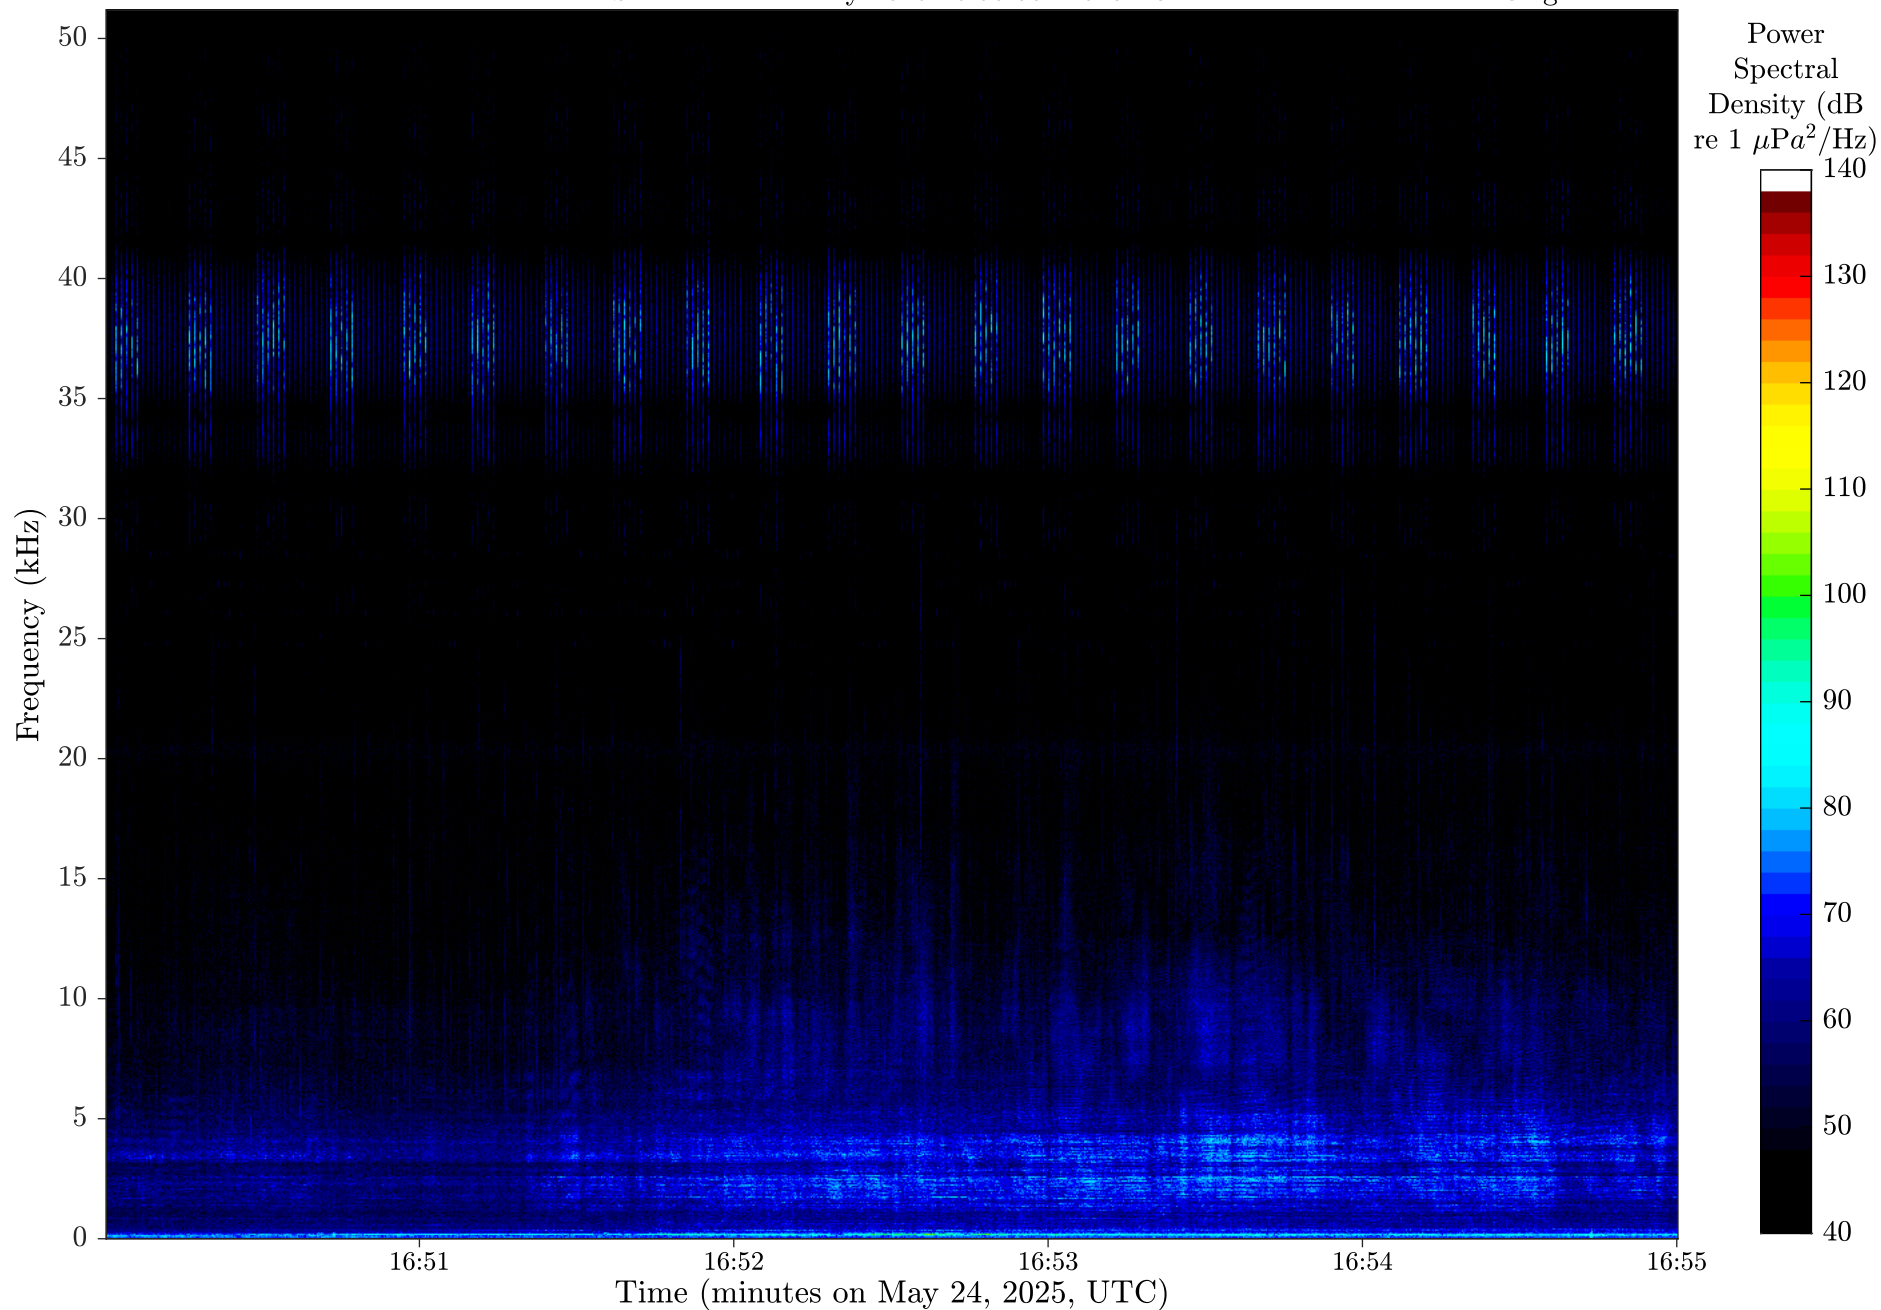

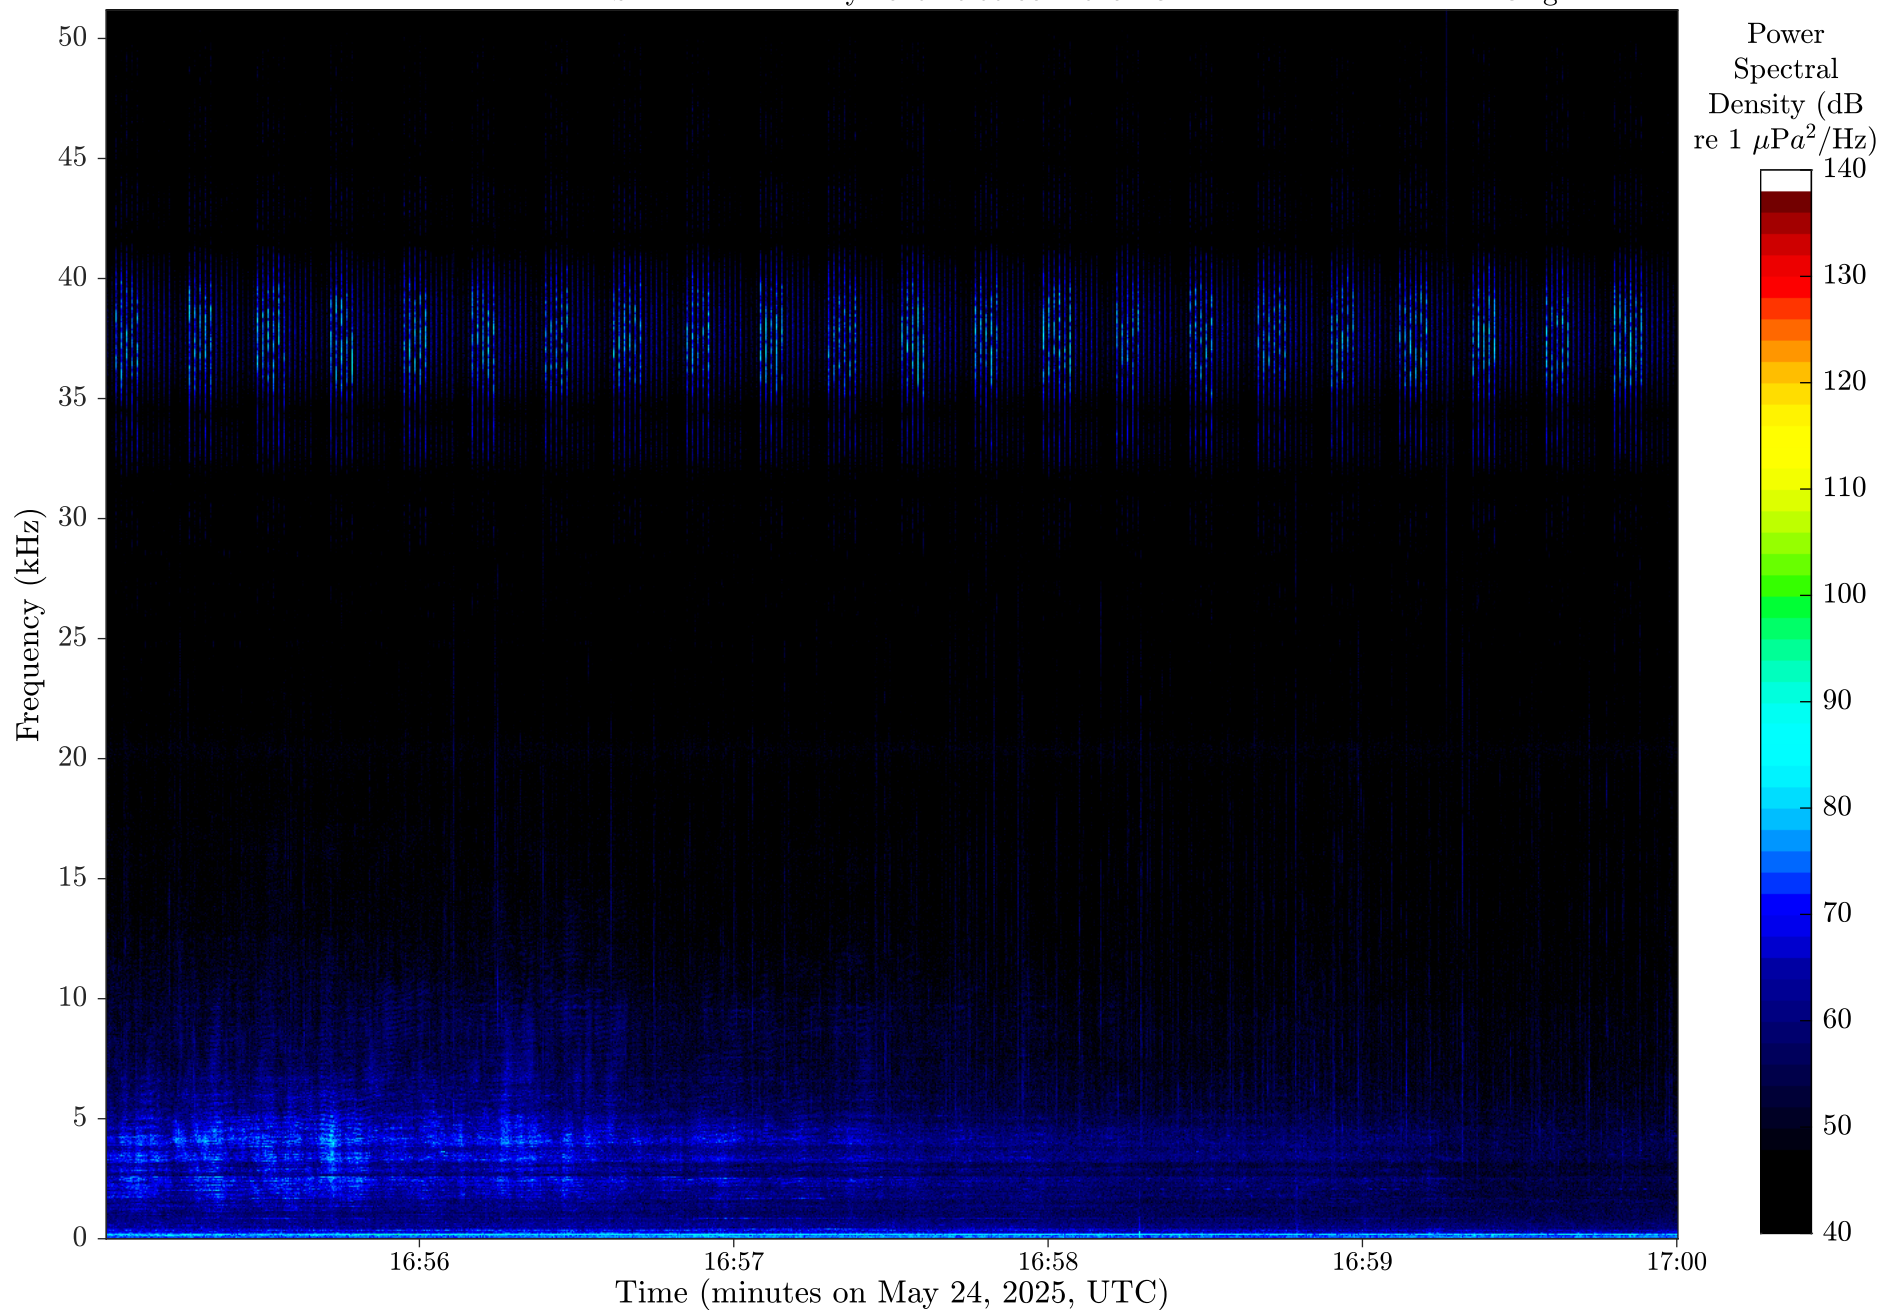


Comments: 28.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:36 UTC

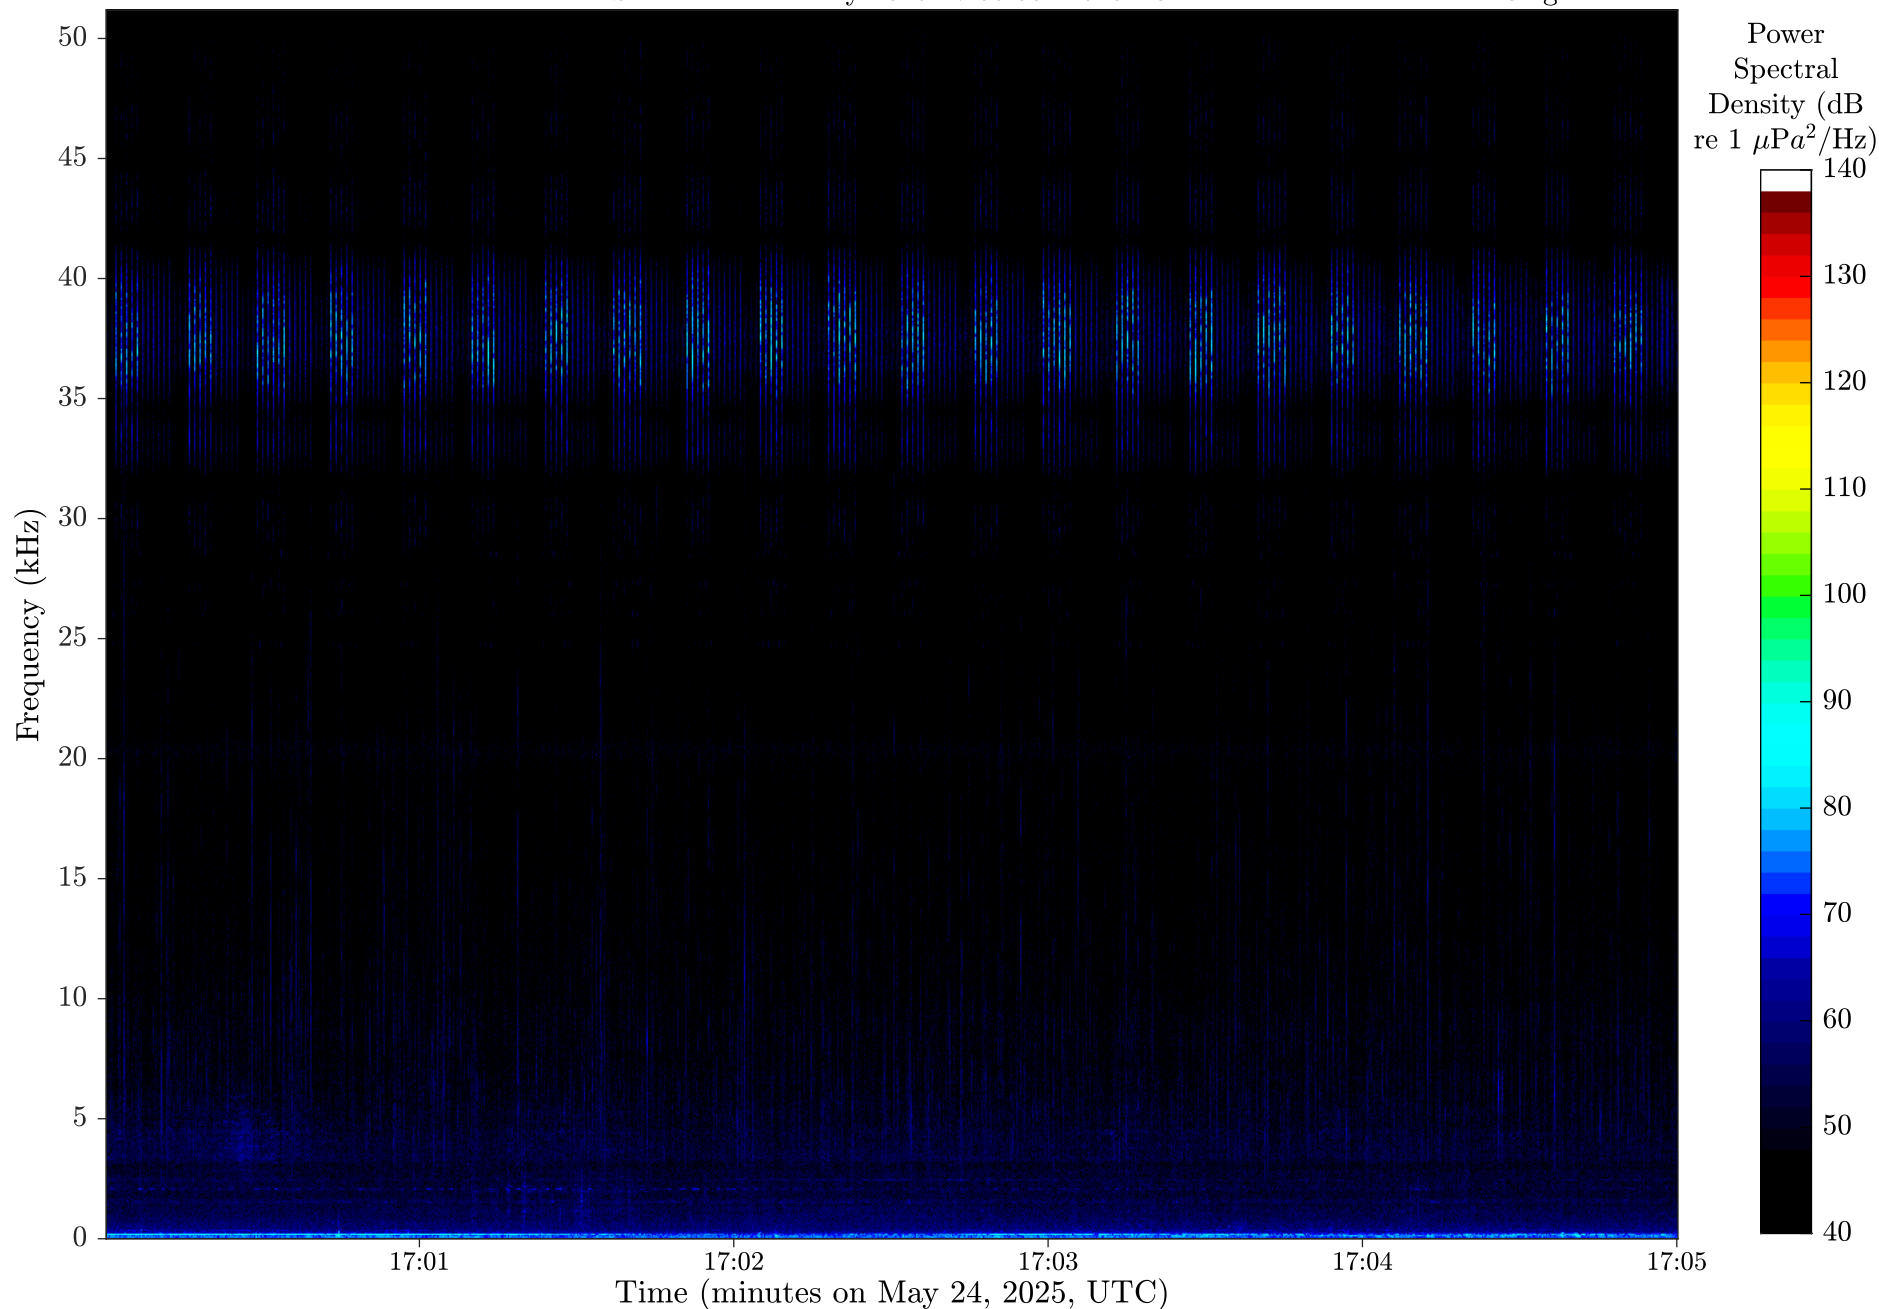


Comments: 28.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:44 UTC

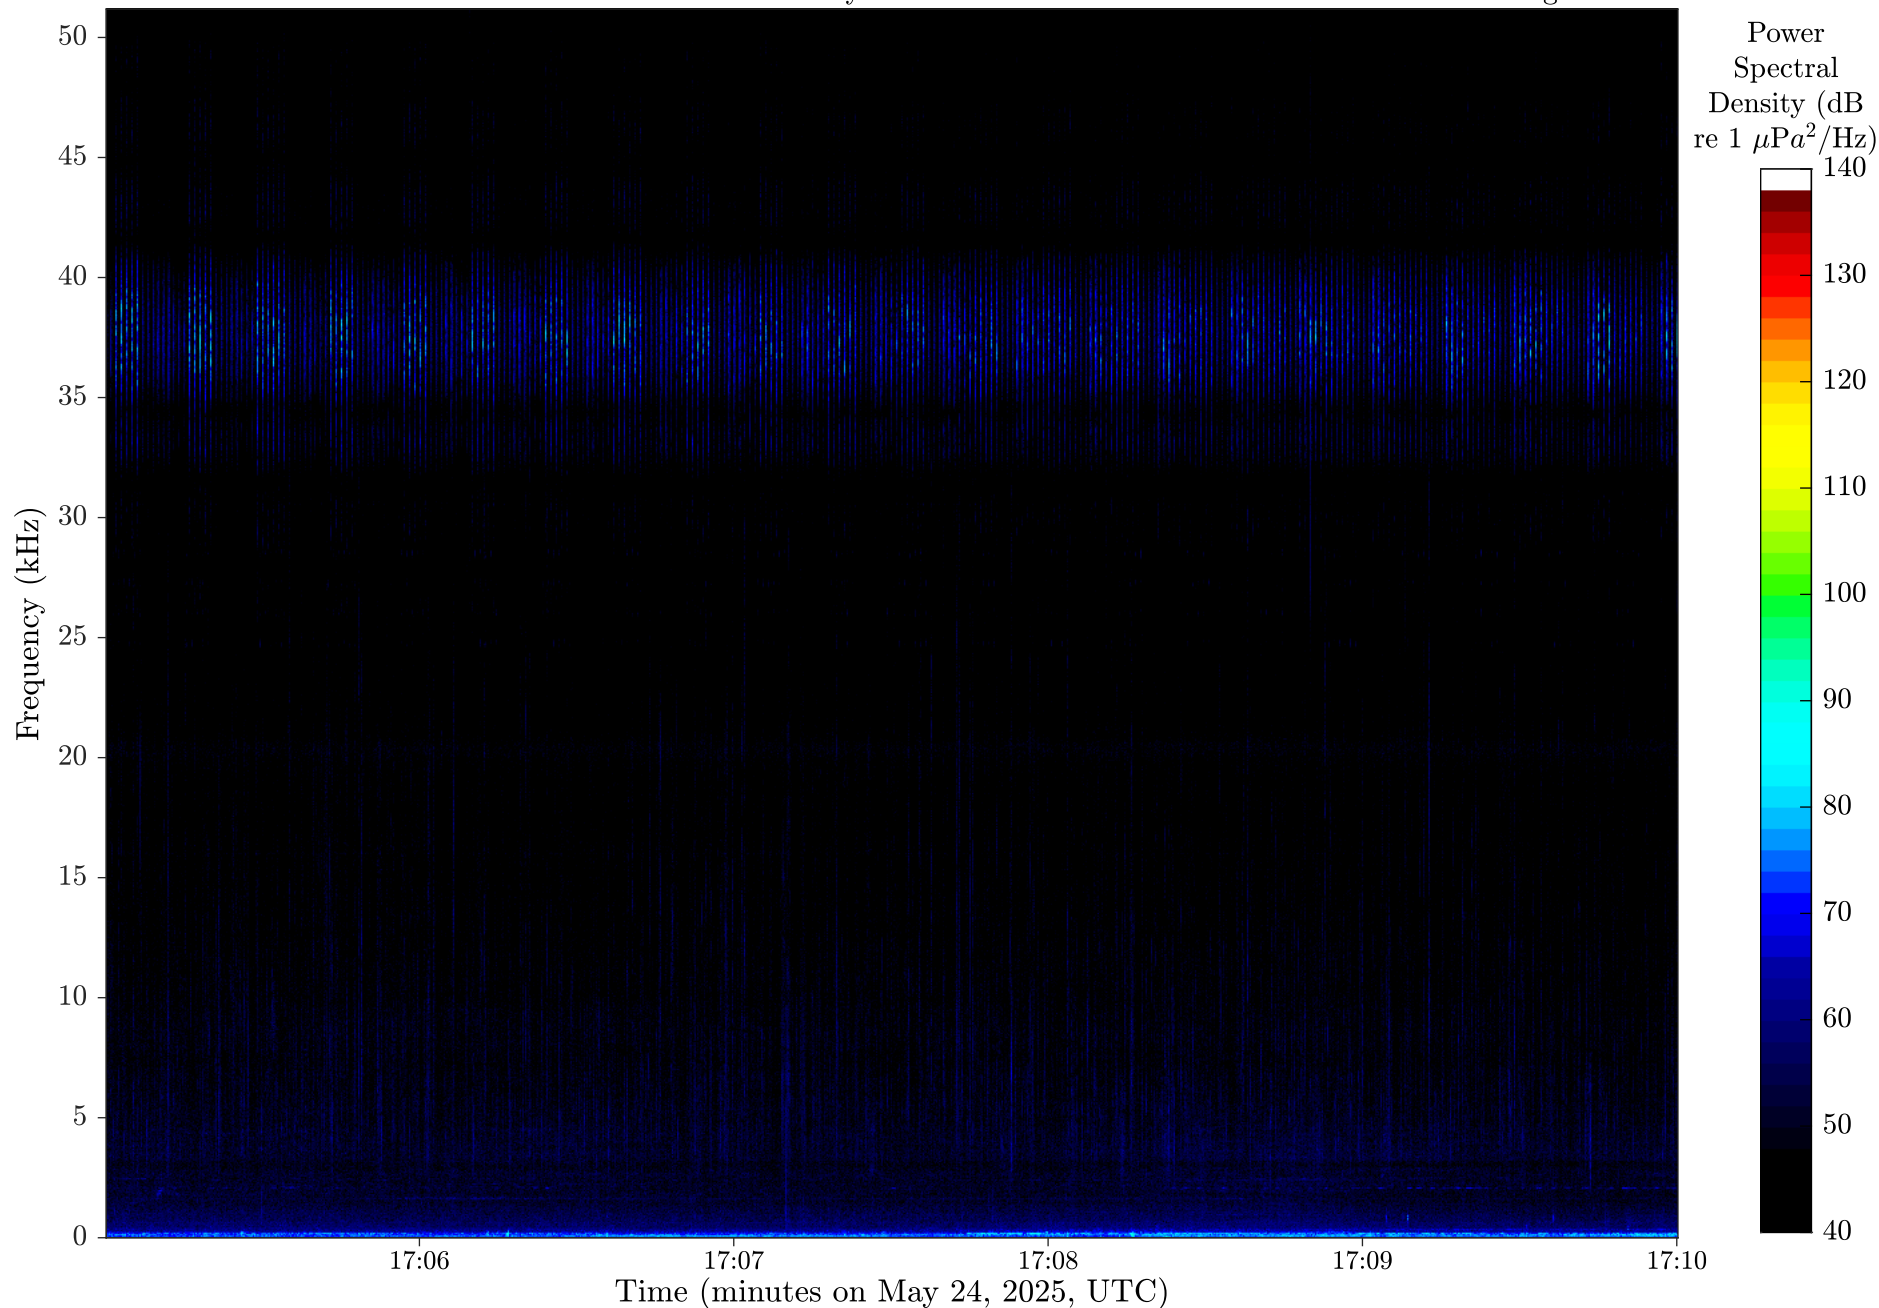


Comments: 28.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:46:52 UTC

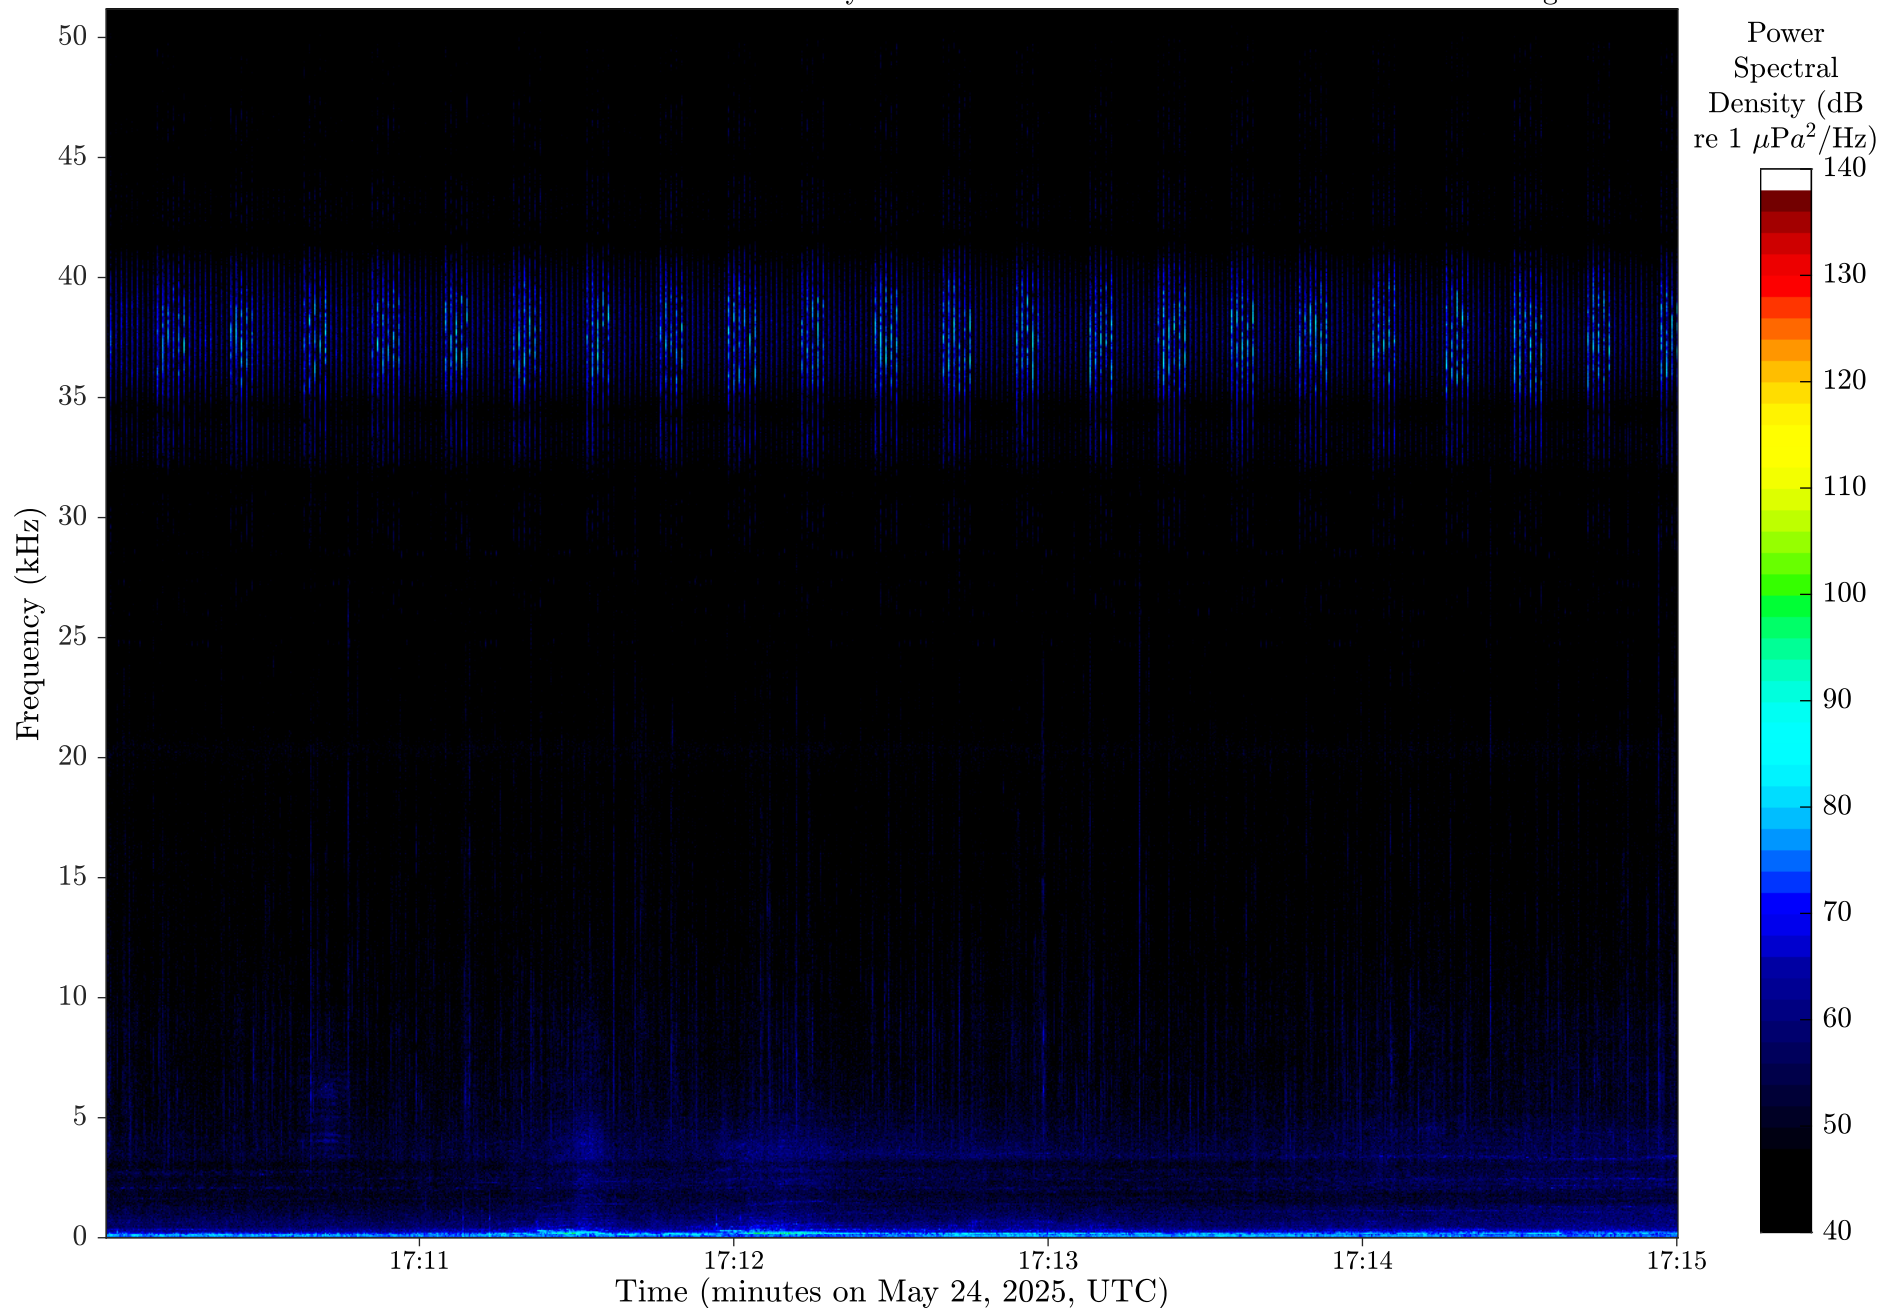


Comments: 30.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:47:00 UTC

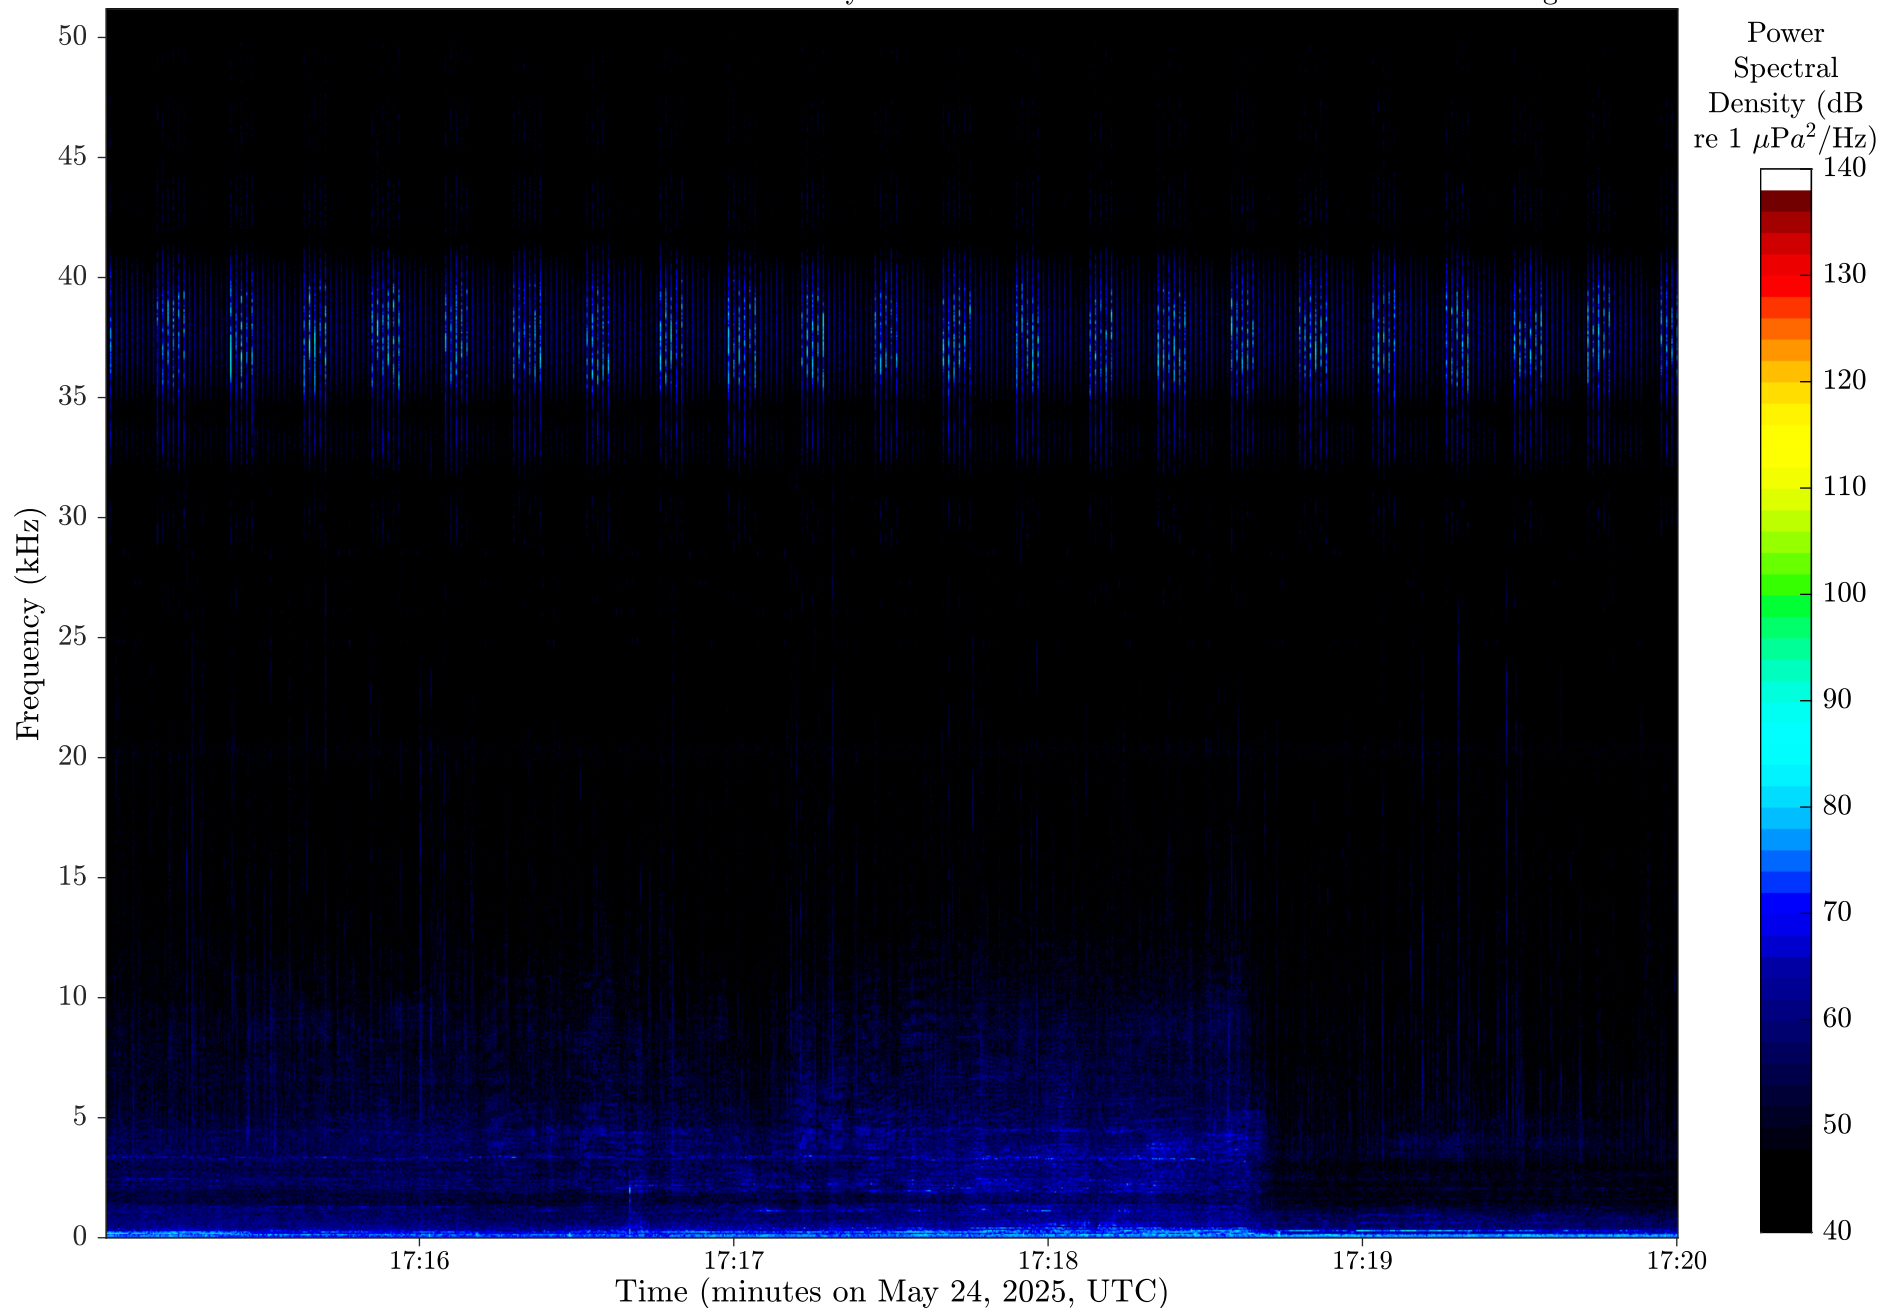


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:47:08 UTC

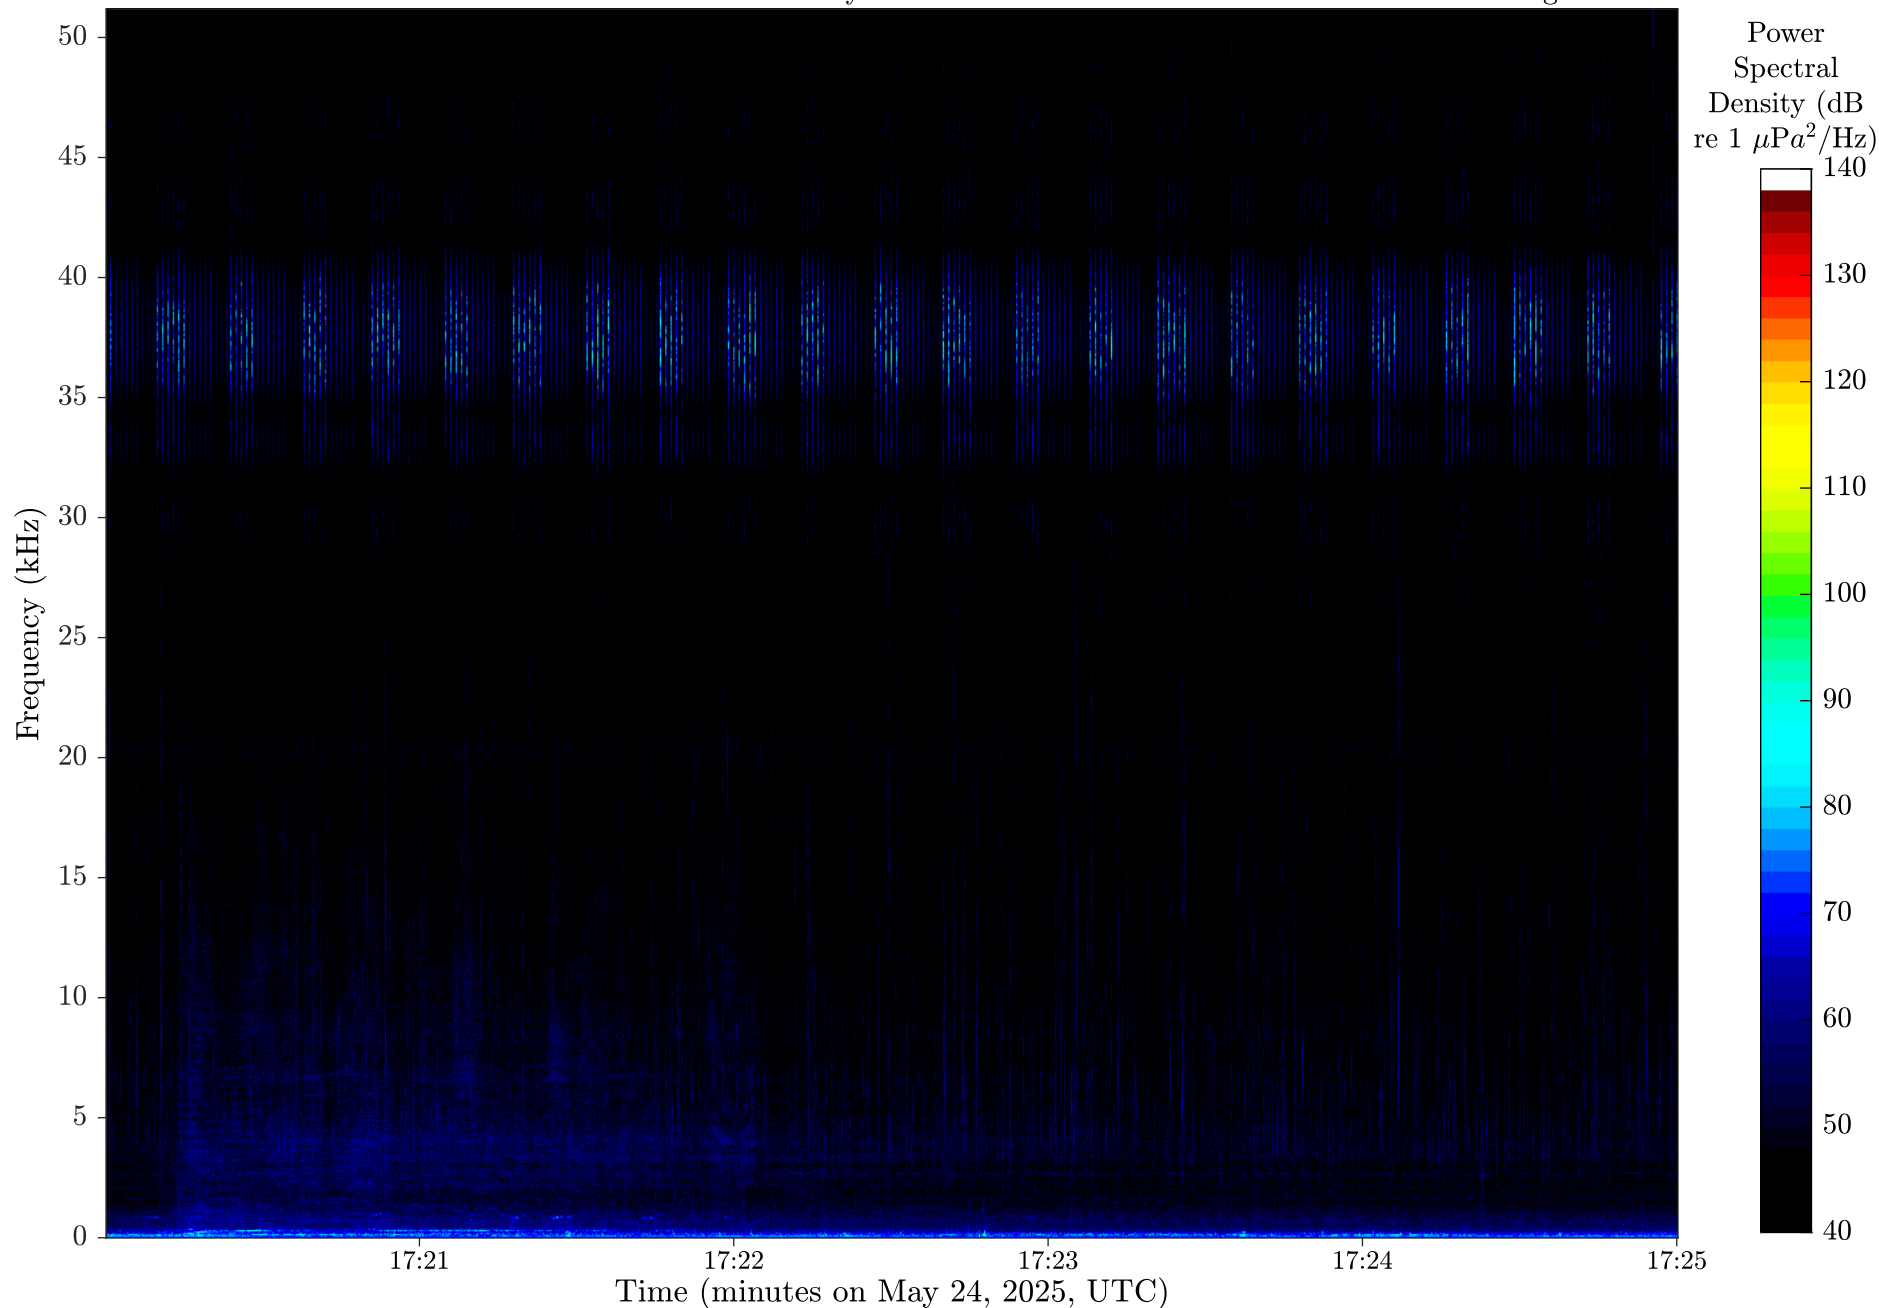


Comments: 32.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:47:16 UTC

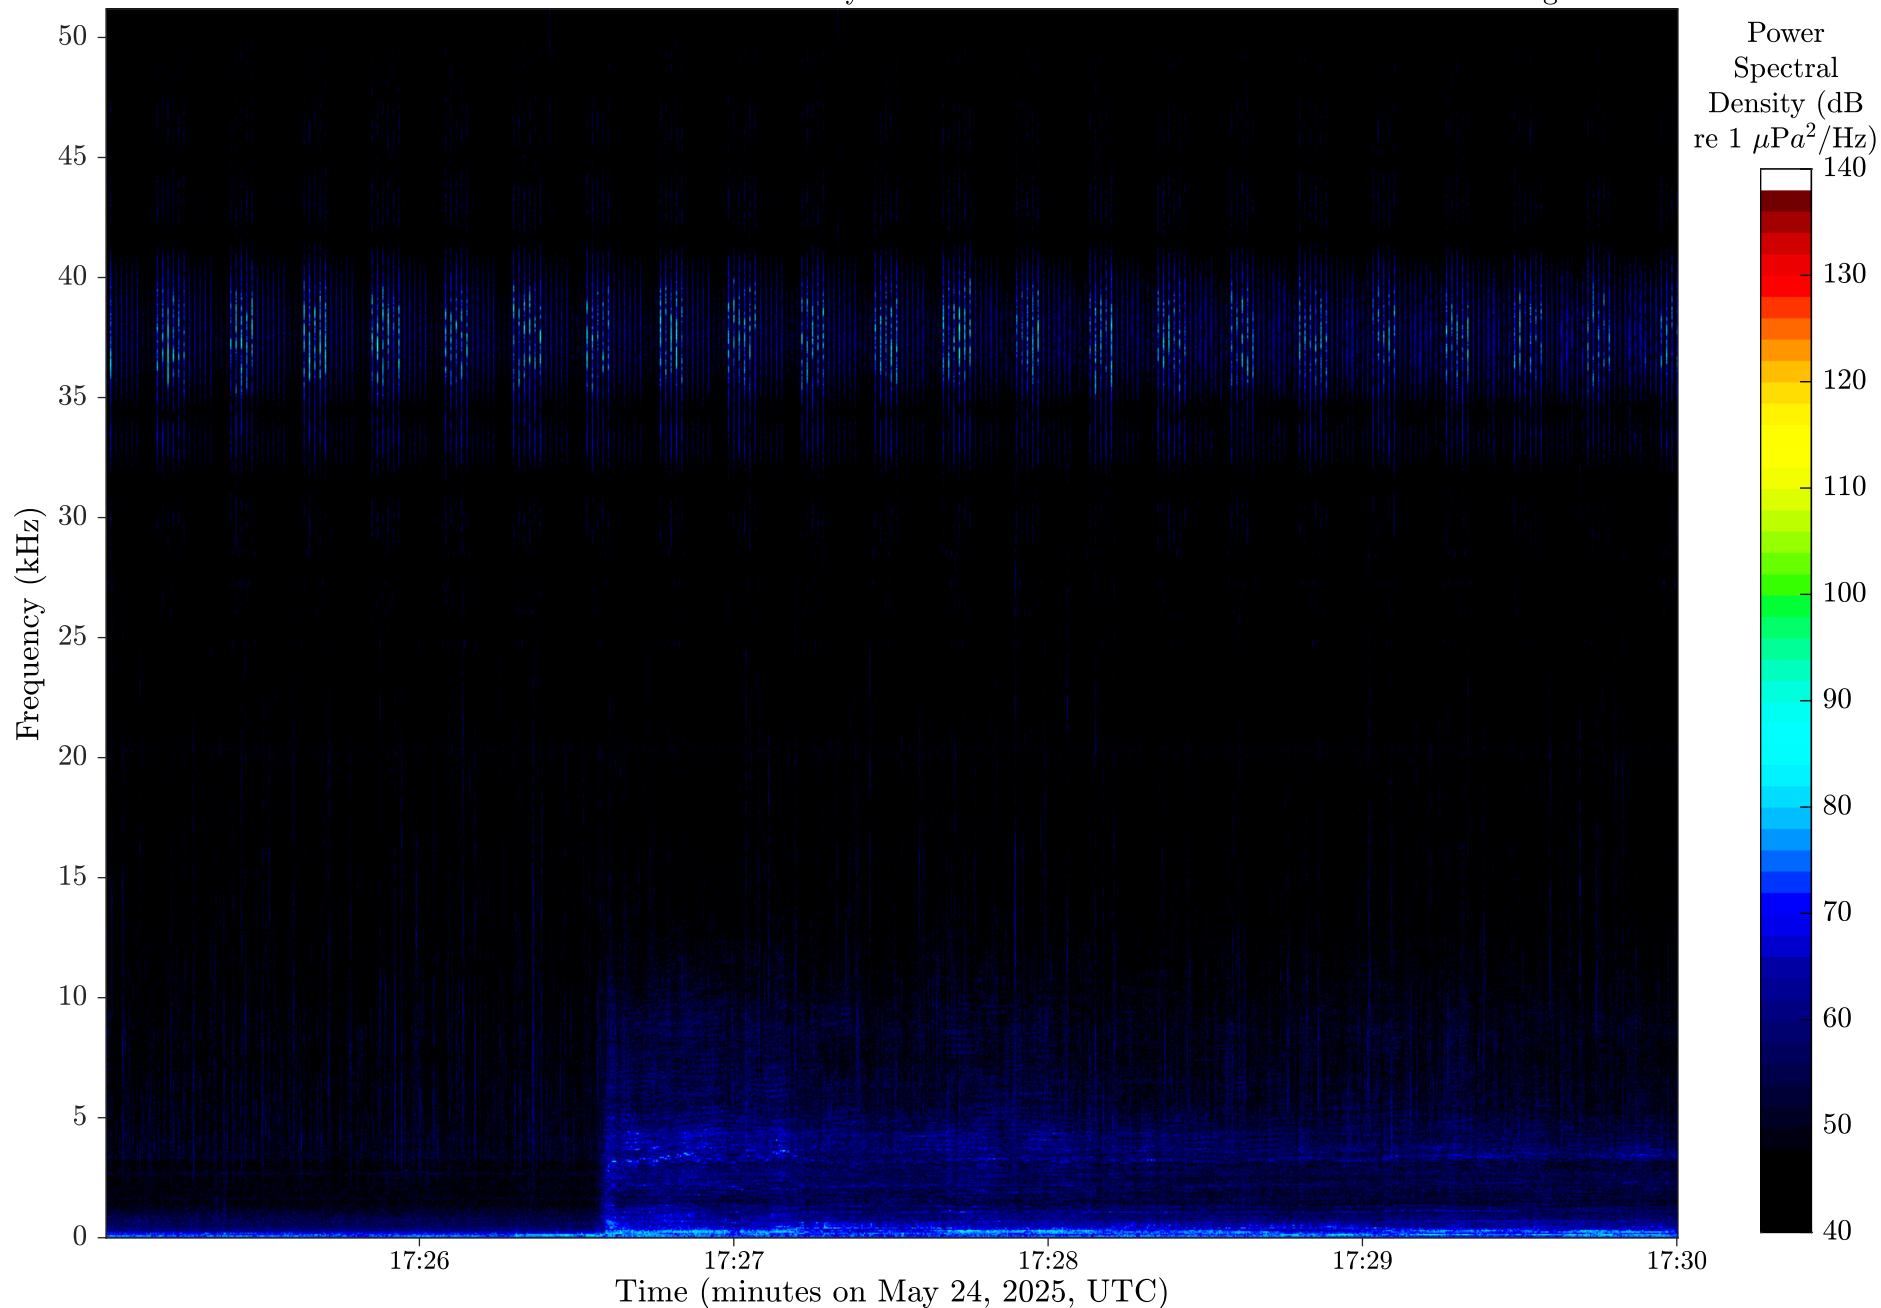


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:47:24 UTC

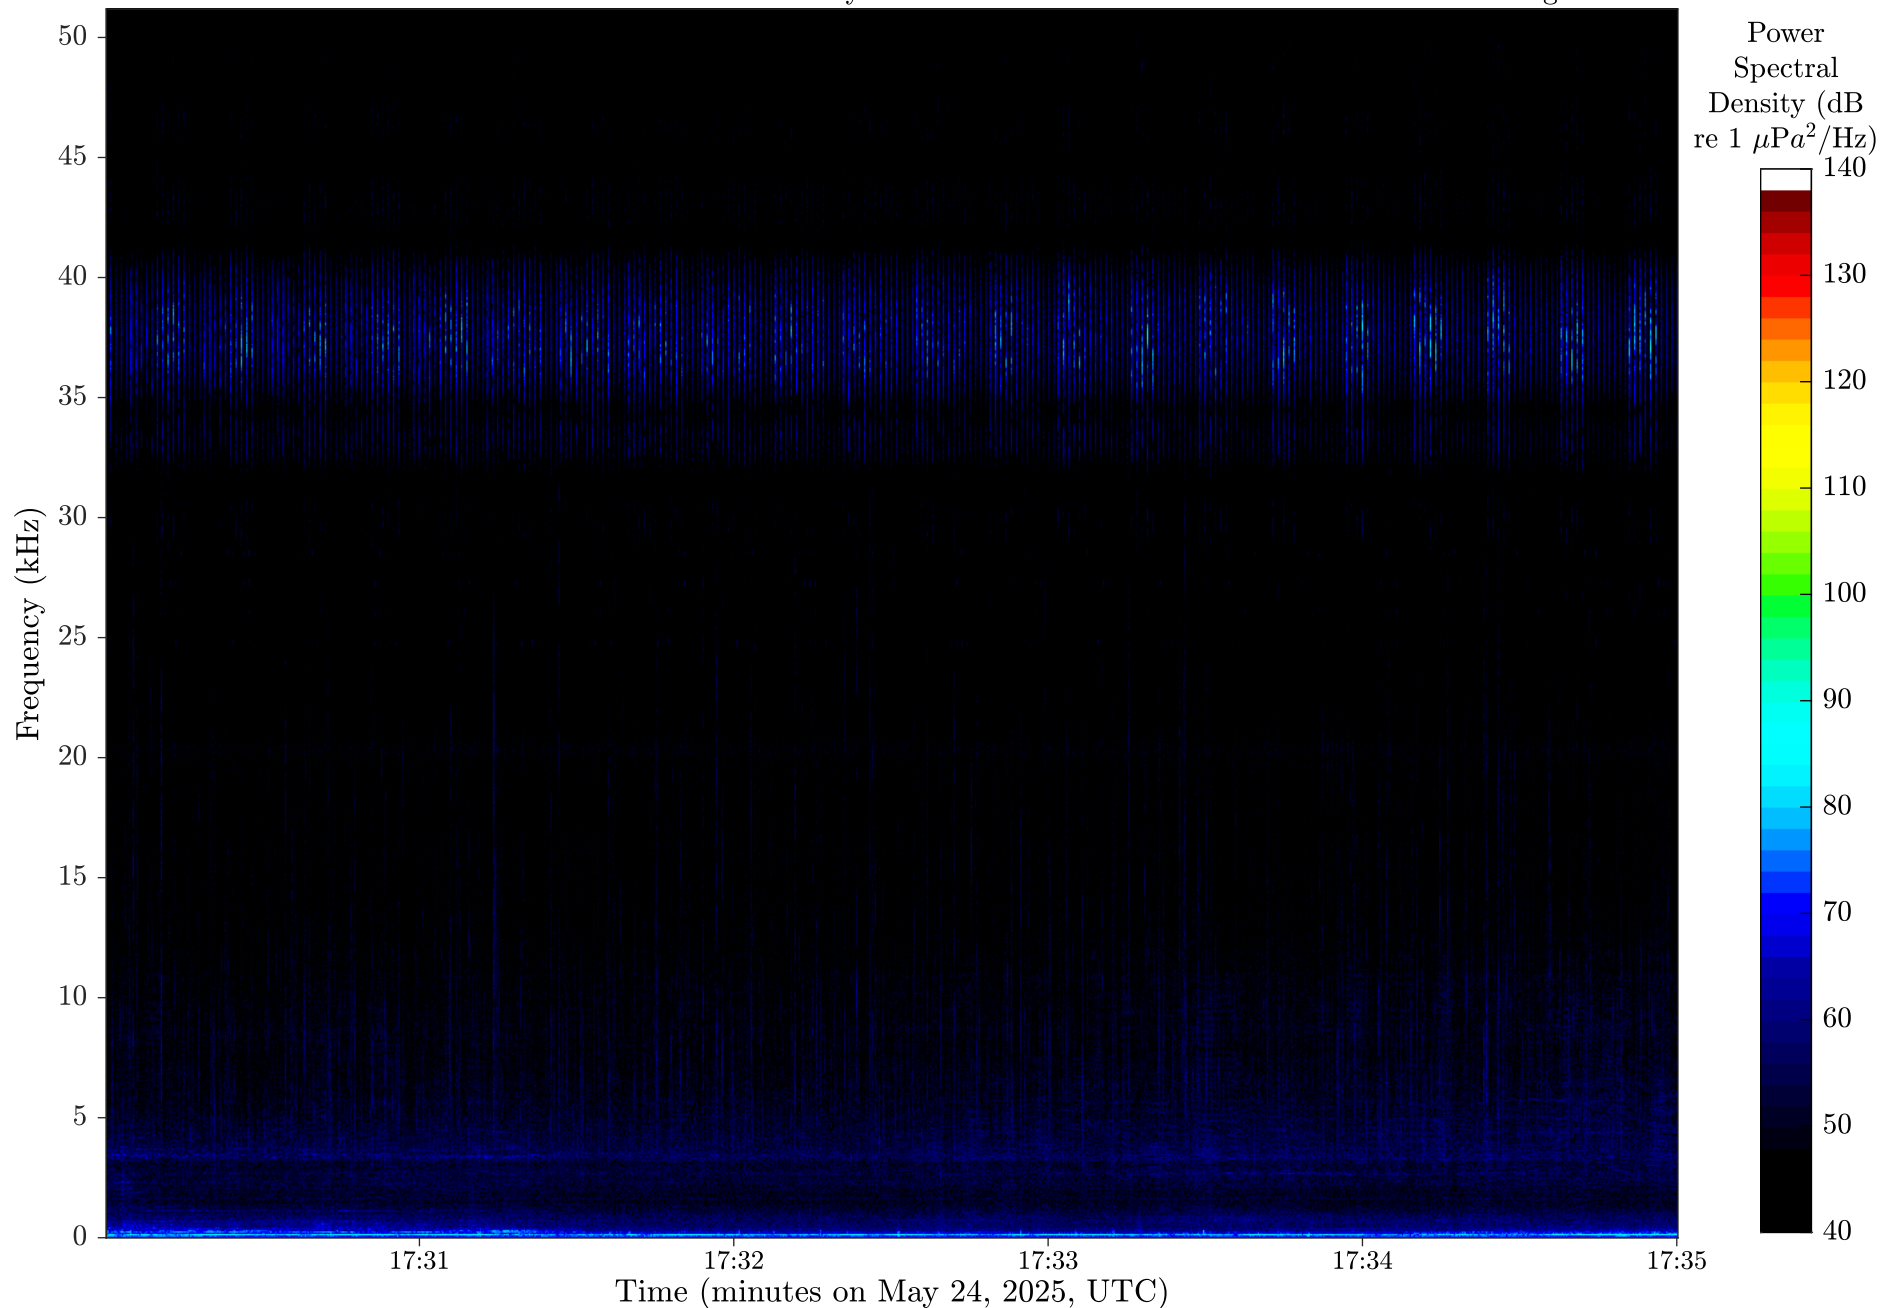


Comments: 31.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:47:32 UTC

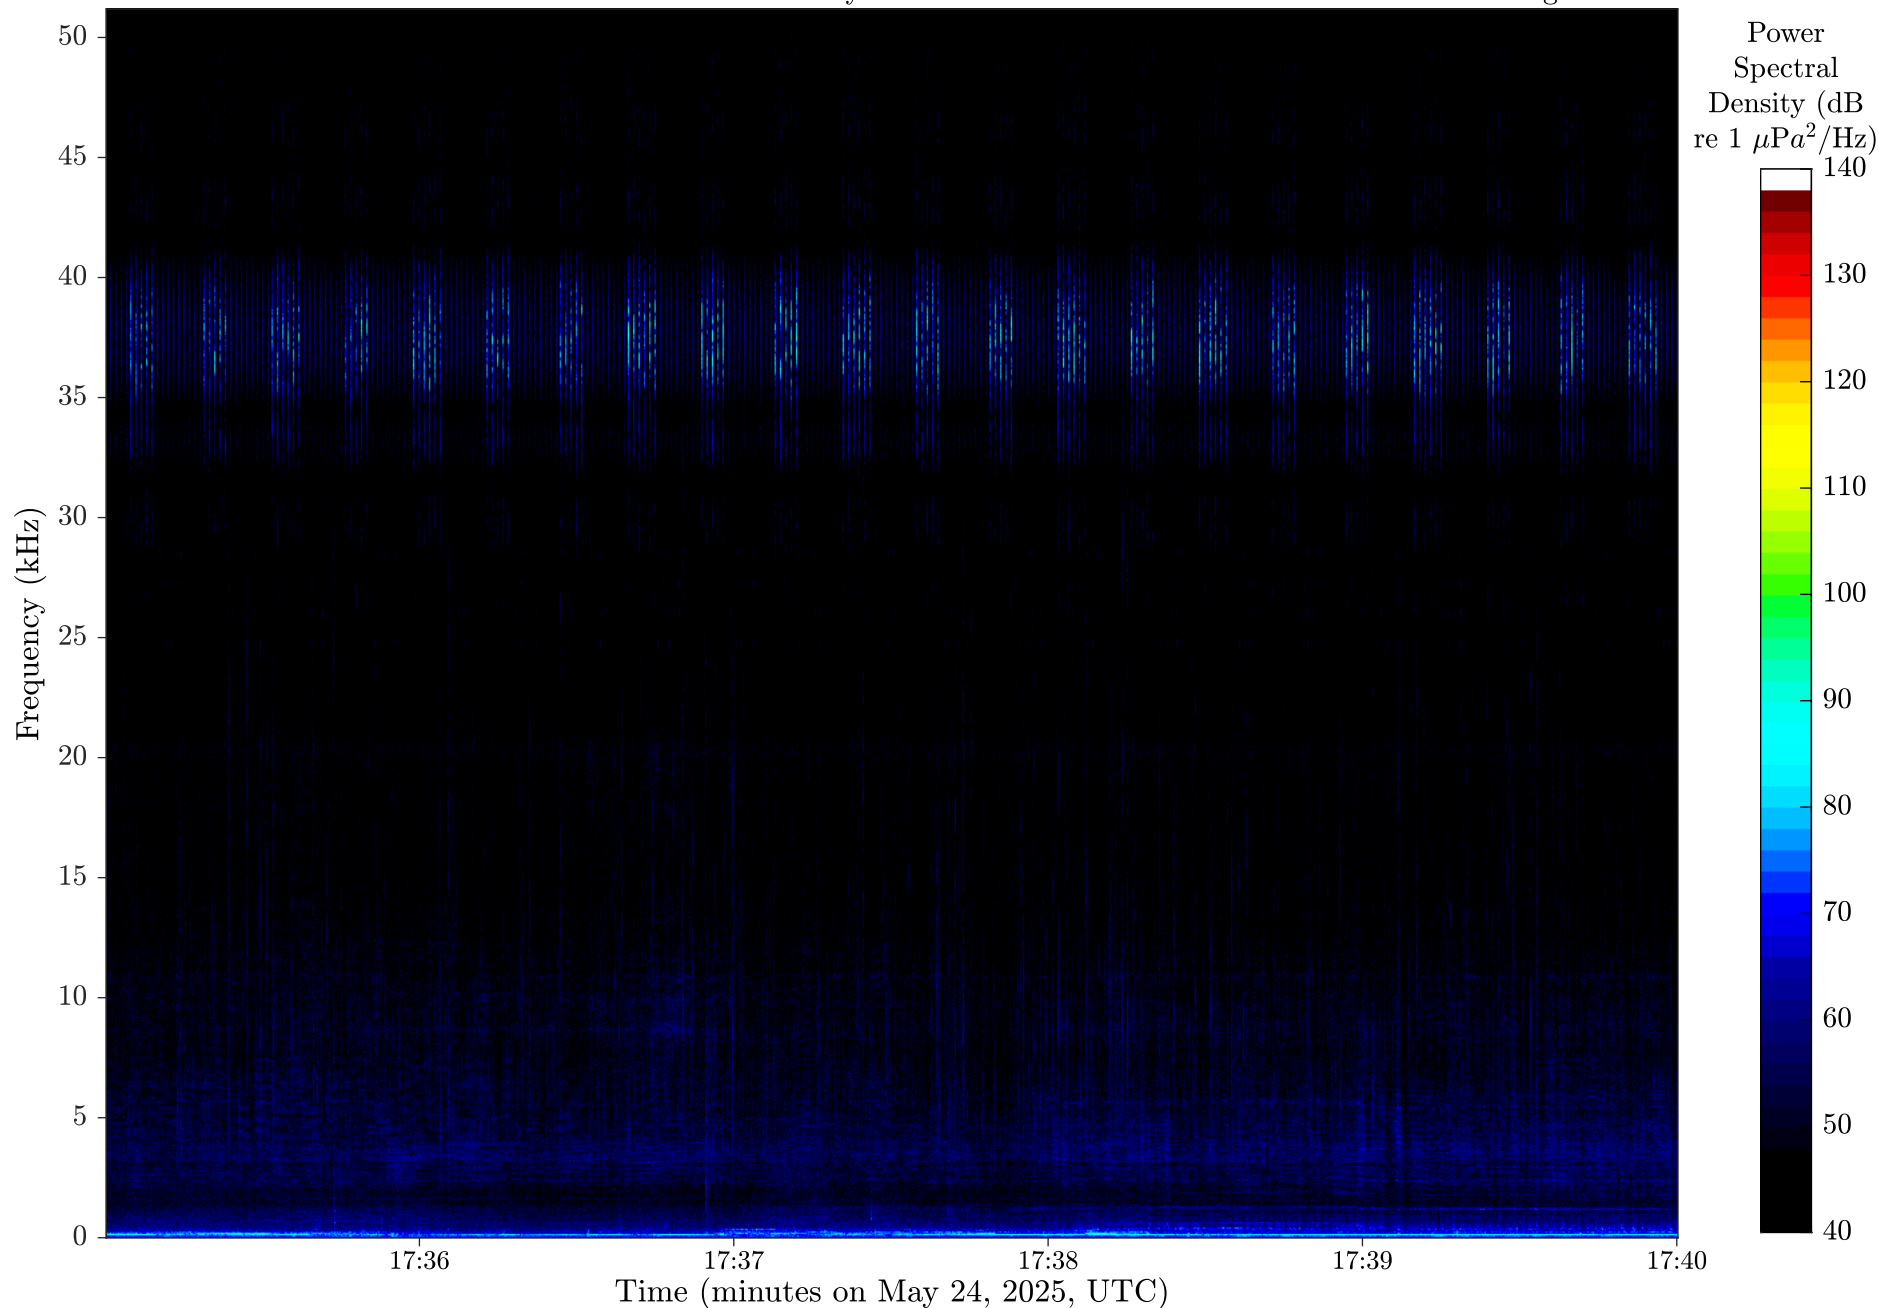


Comments: 30.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:47:40 UTC

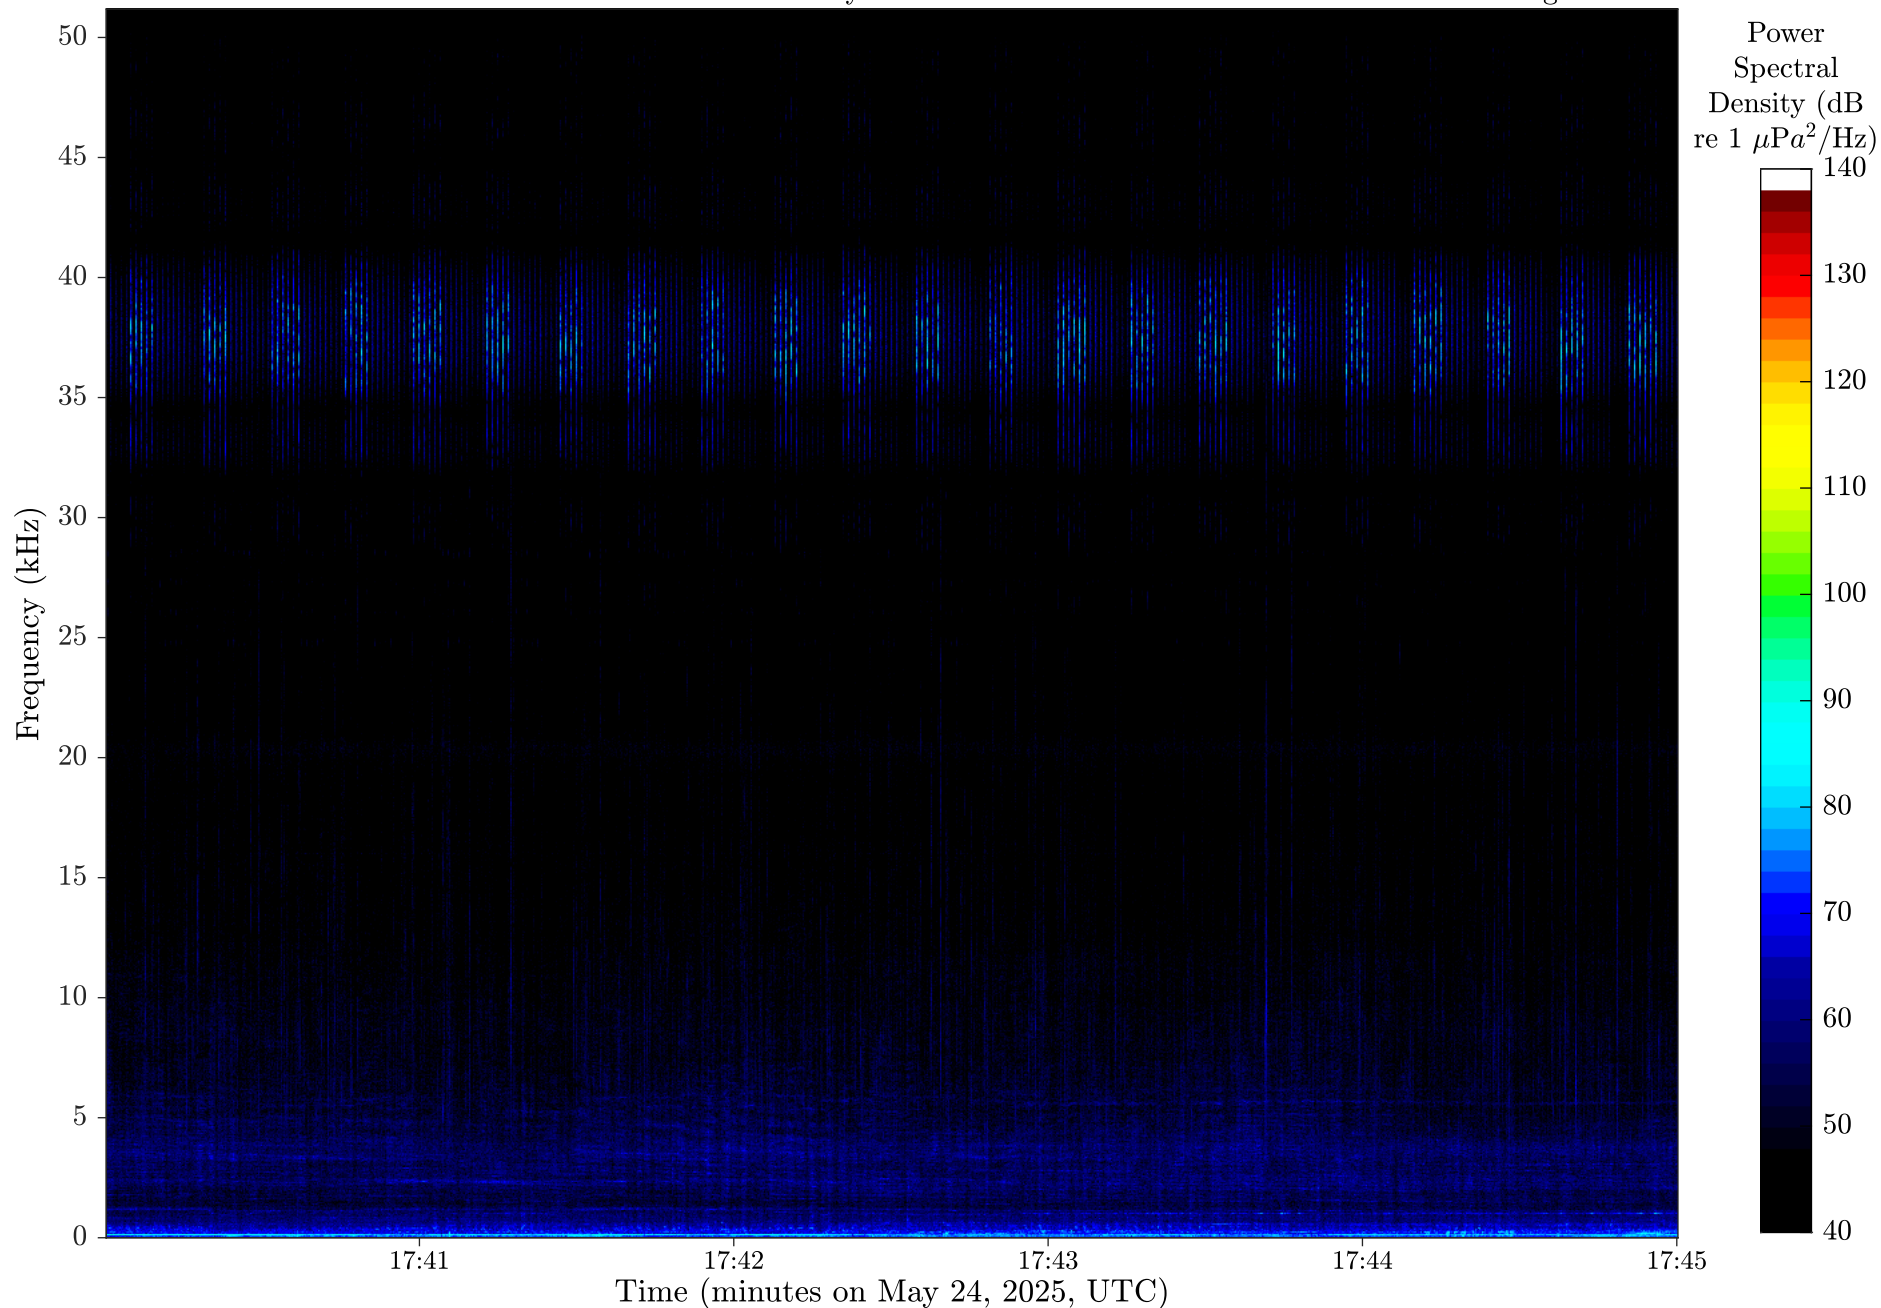


Comments: 32.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:47:49 UTC

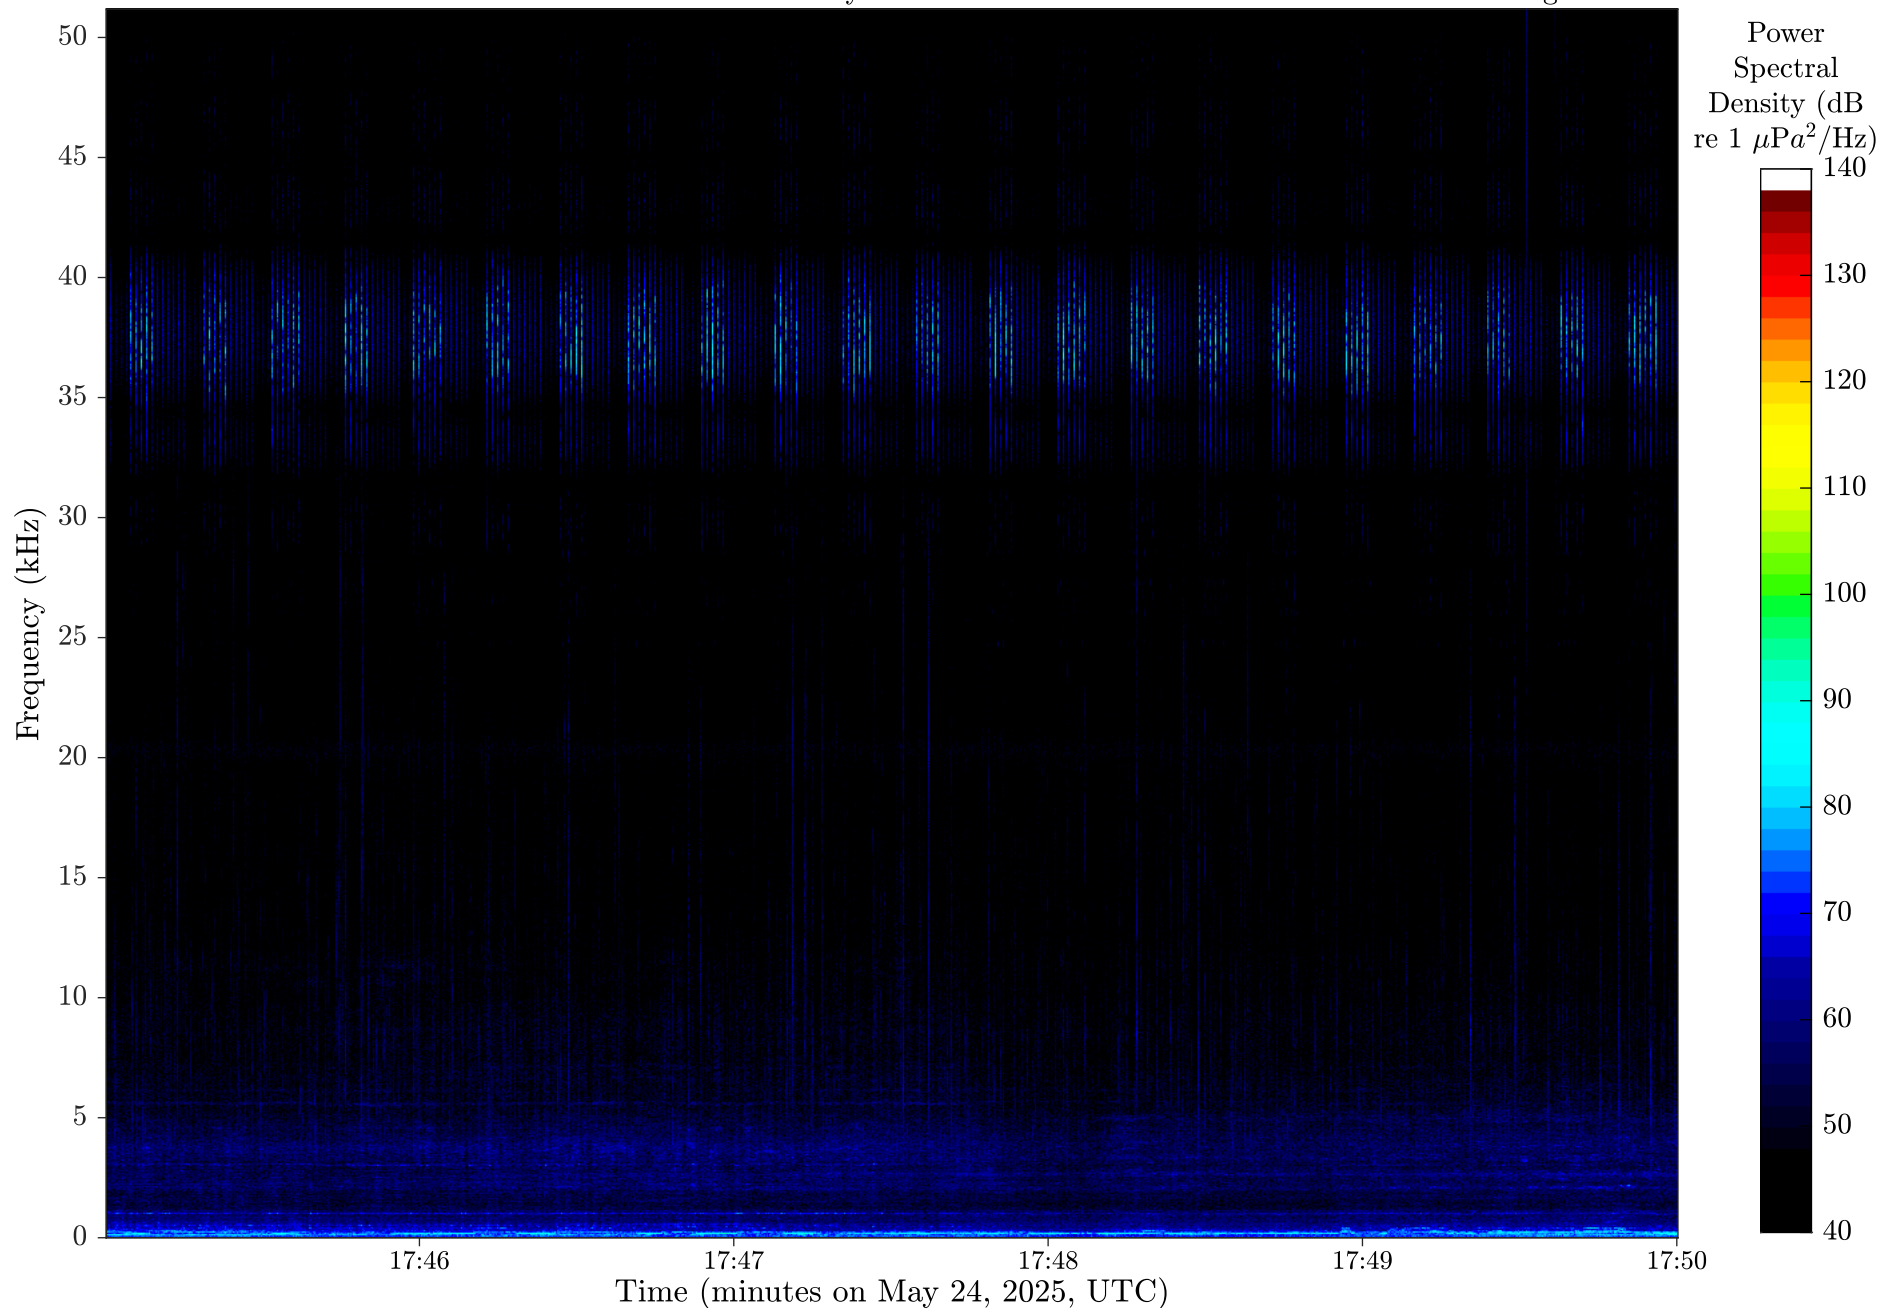


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:47:57 UTC

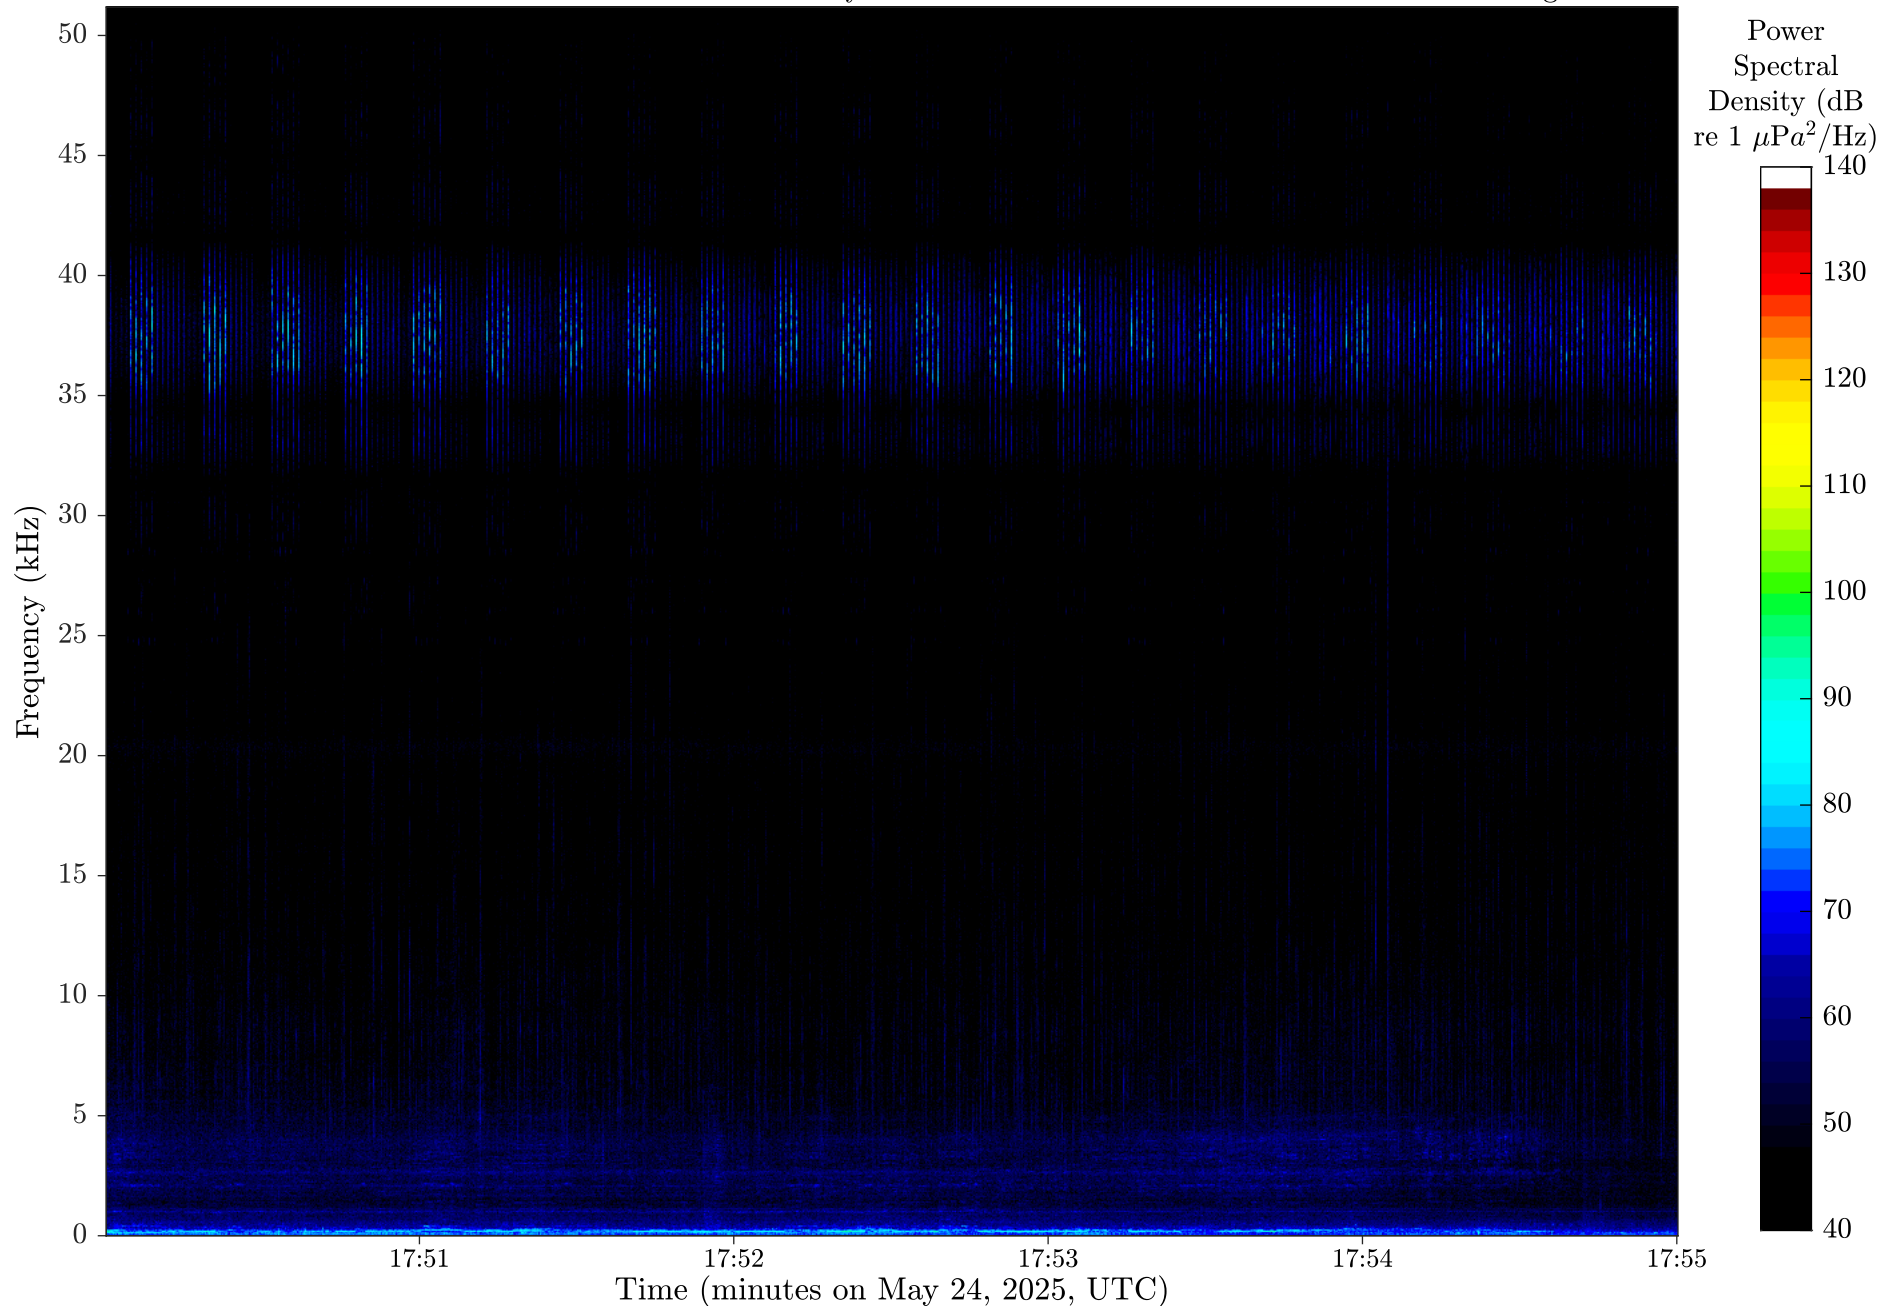


Comments: 32.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:48:05 UTC

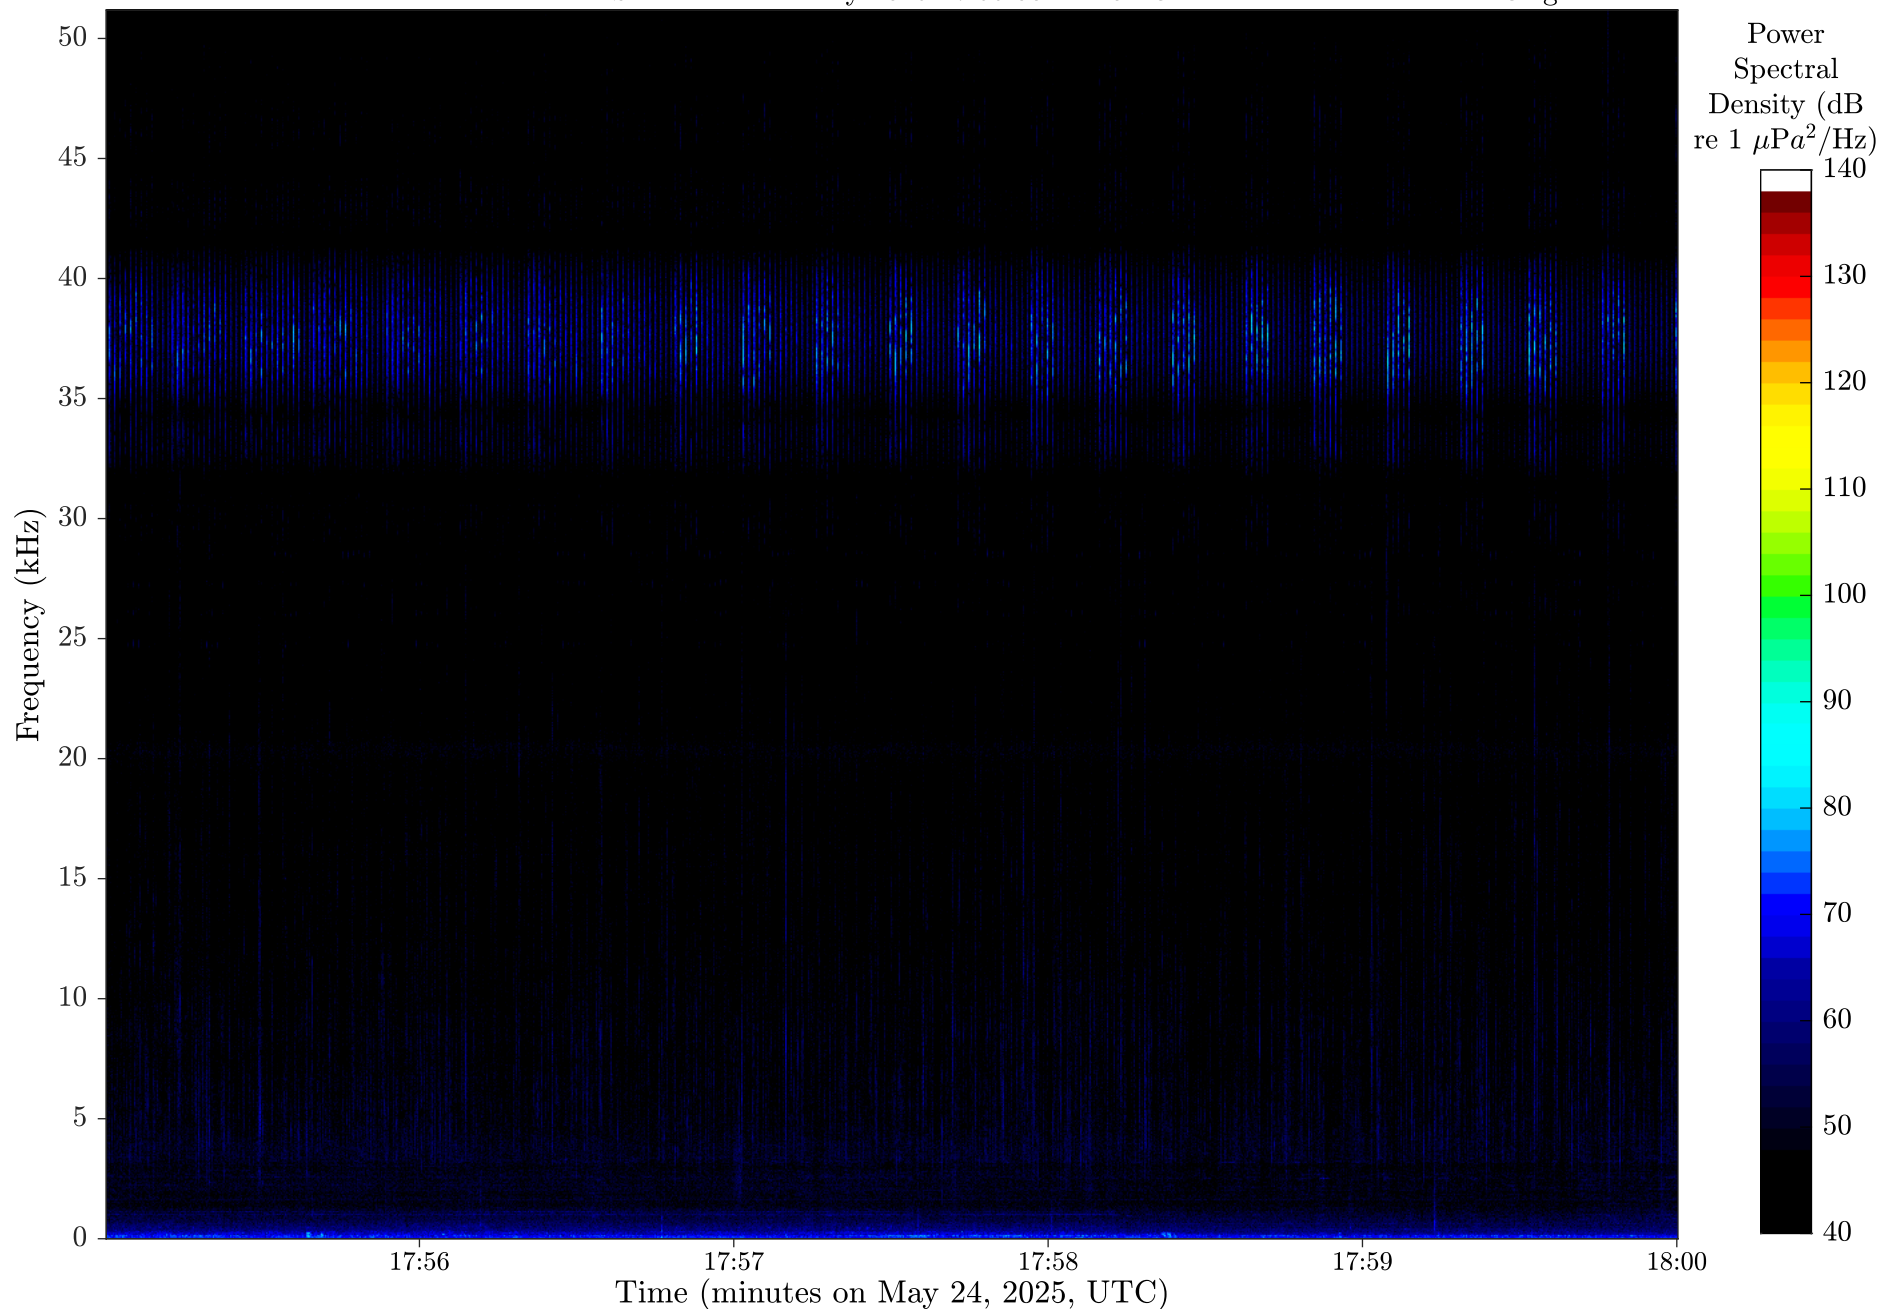


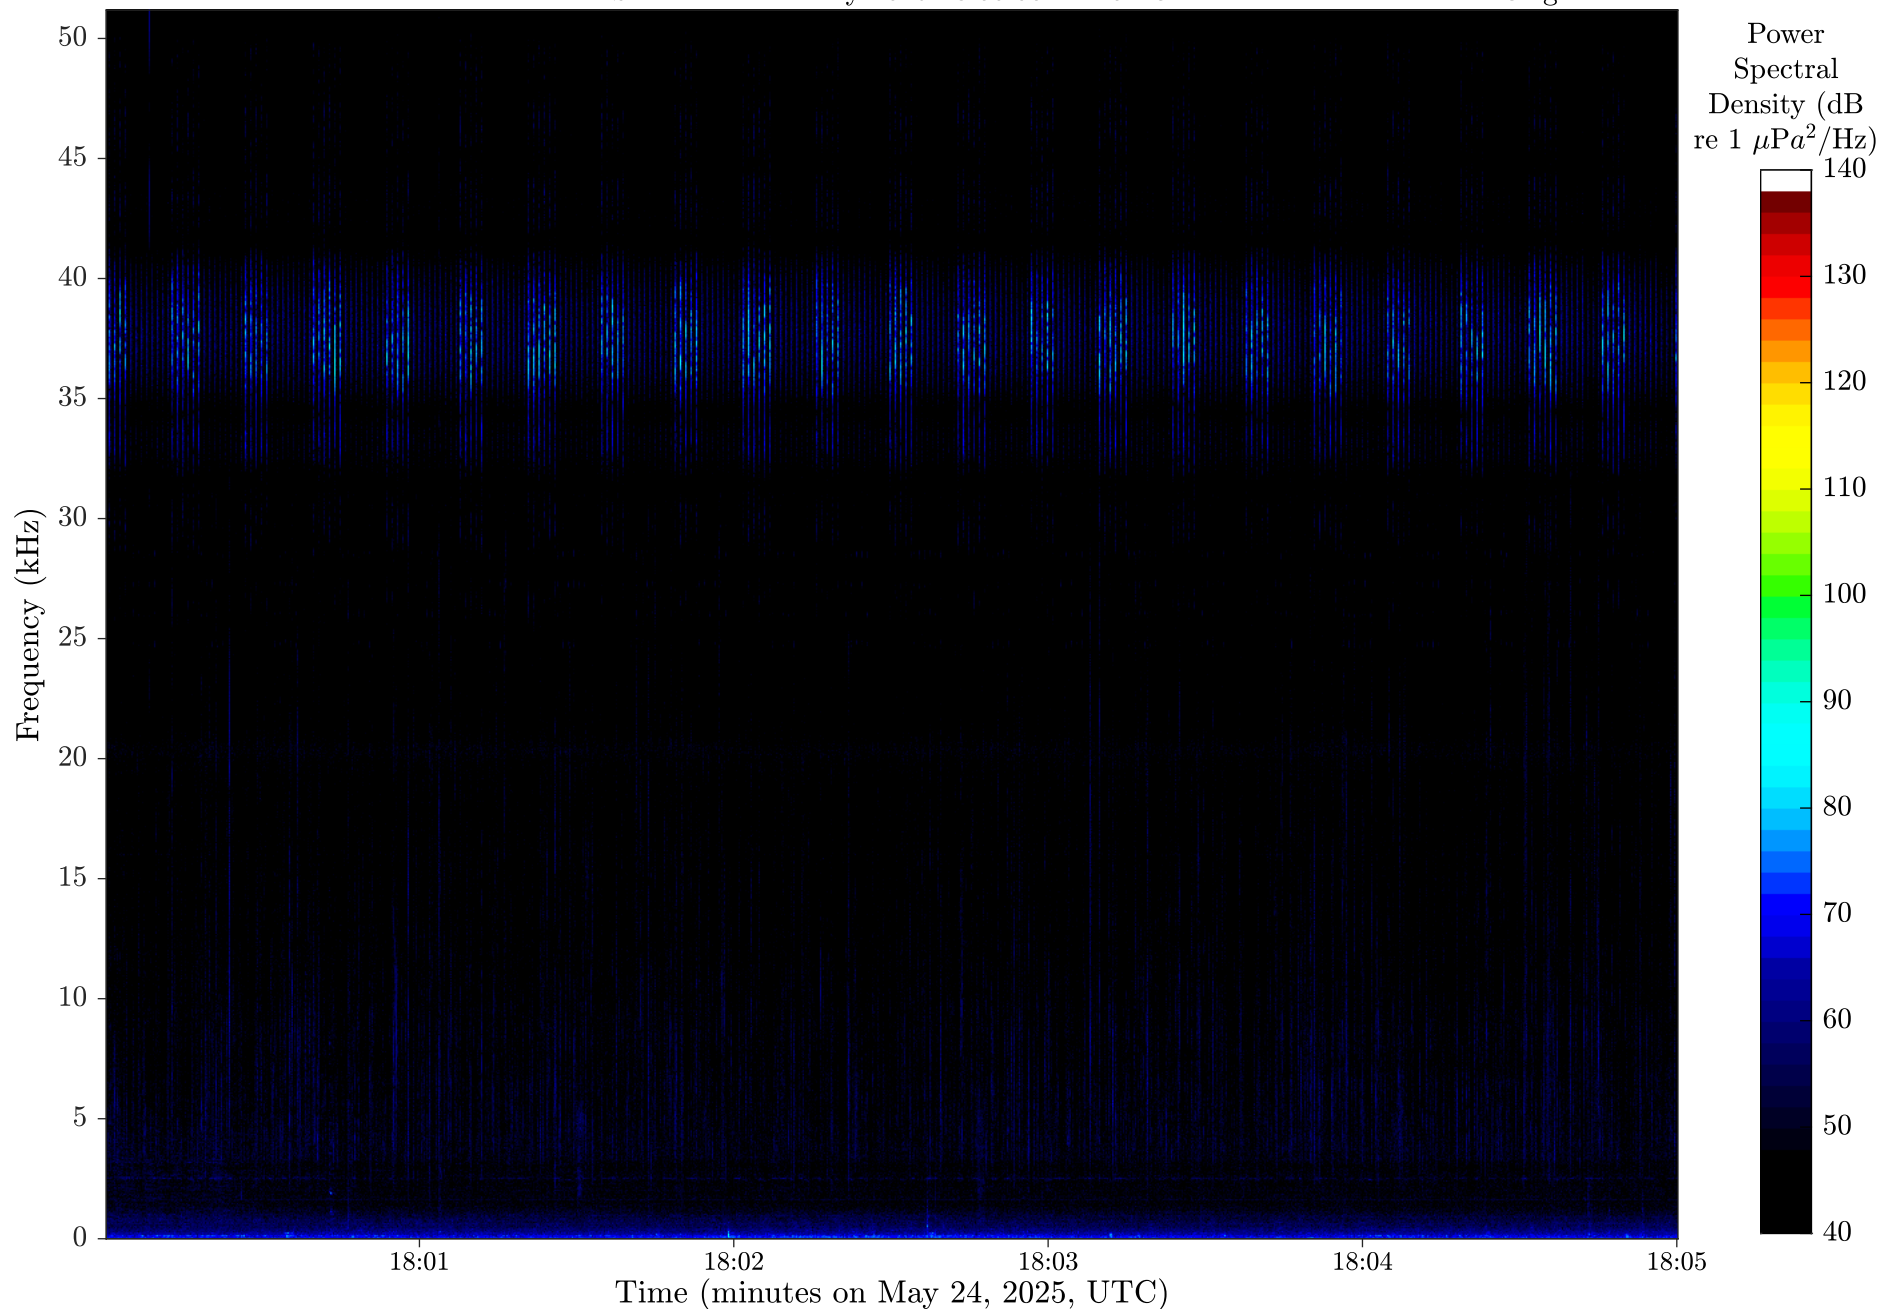


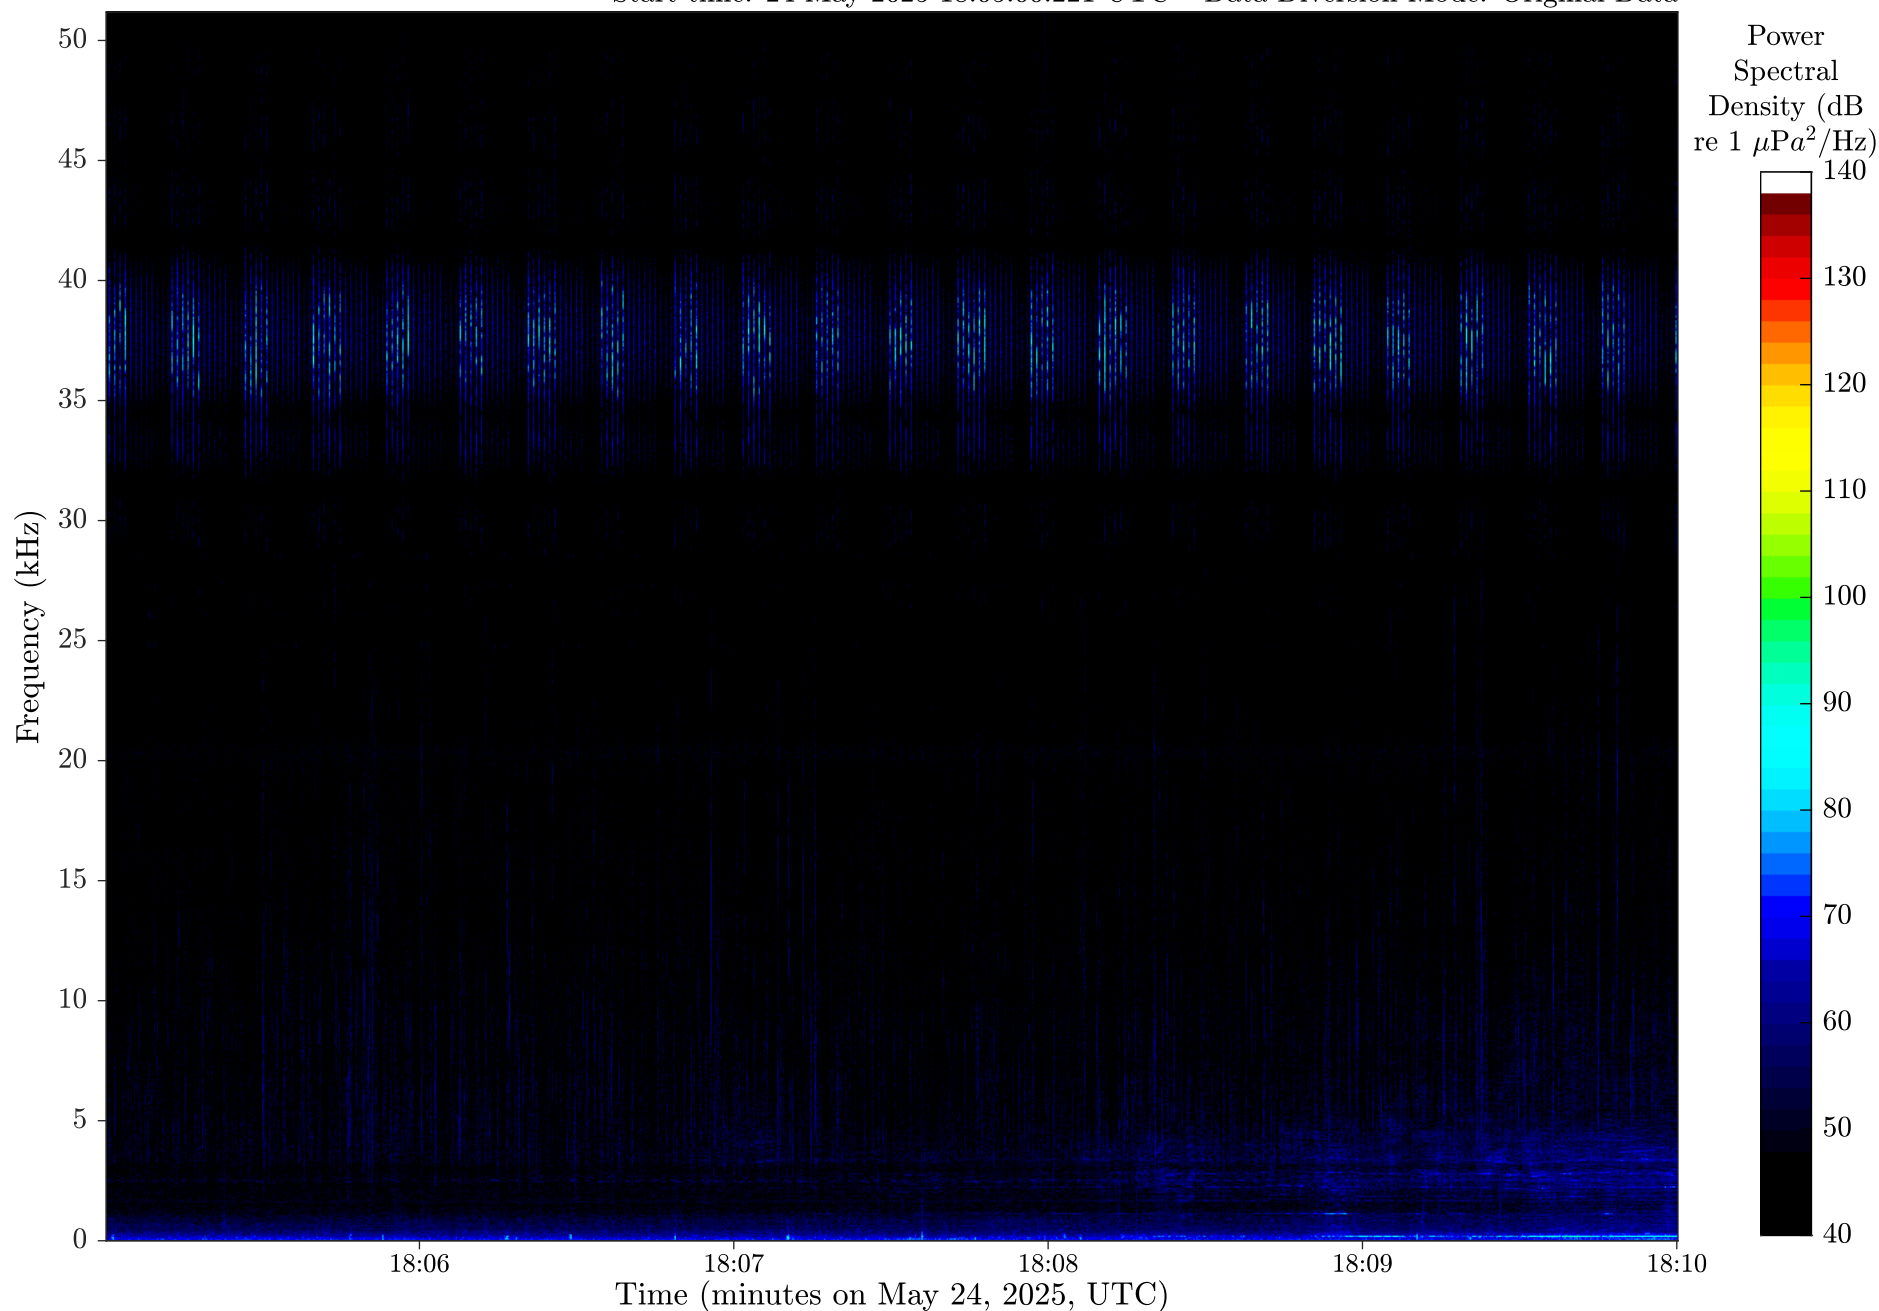

Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:48:31 UTC

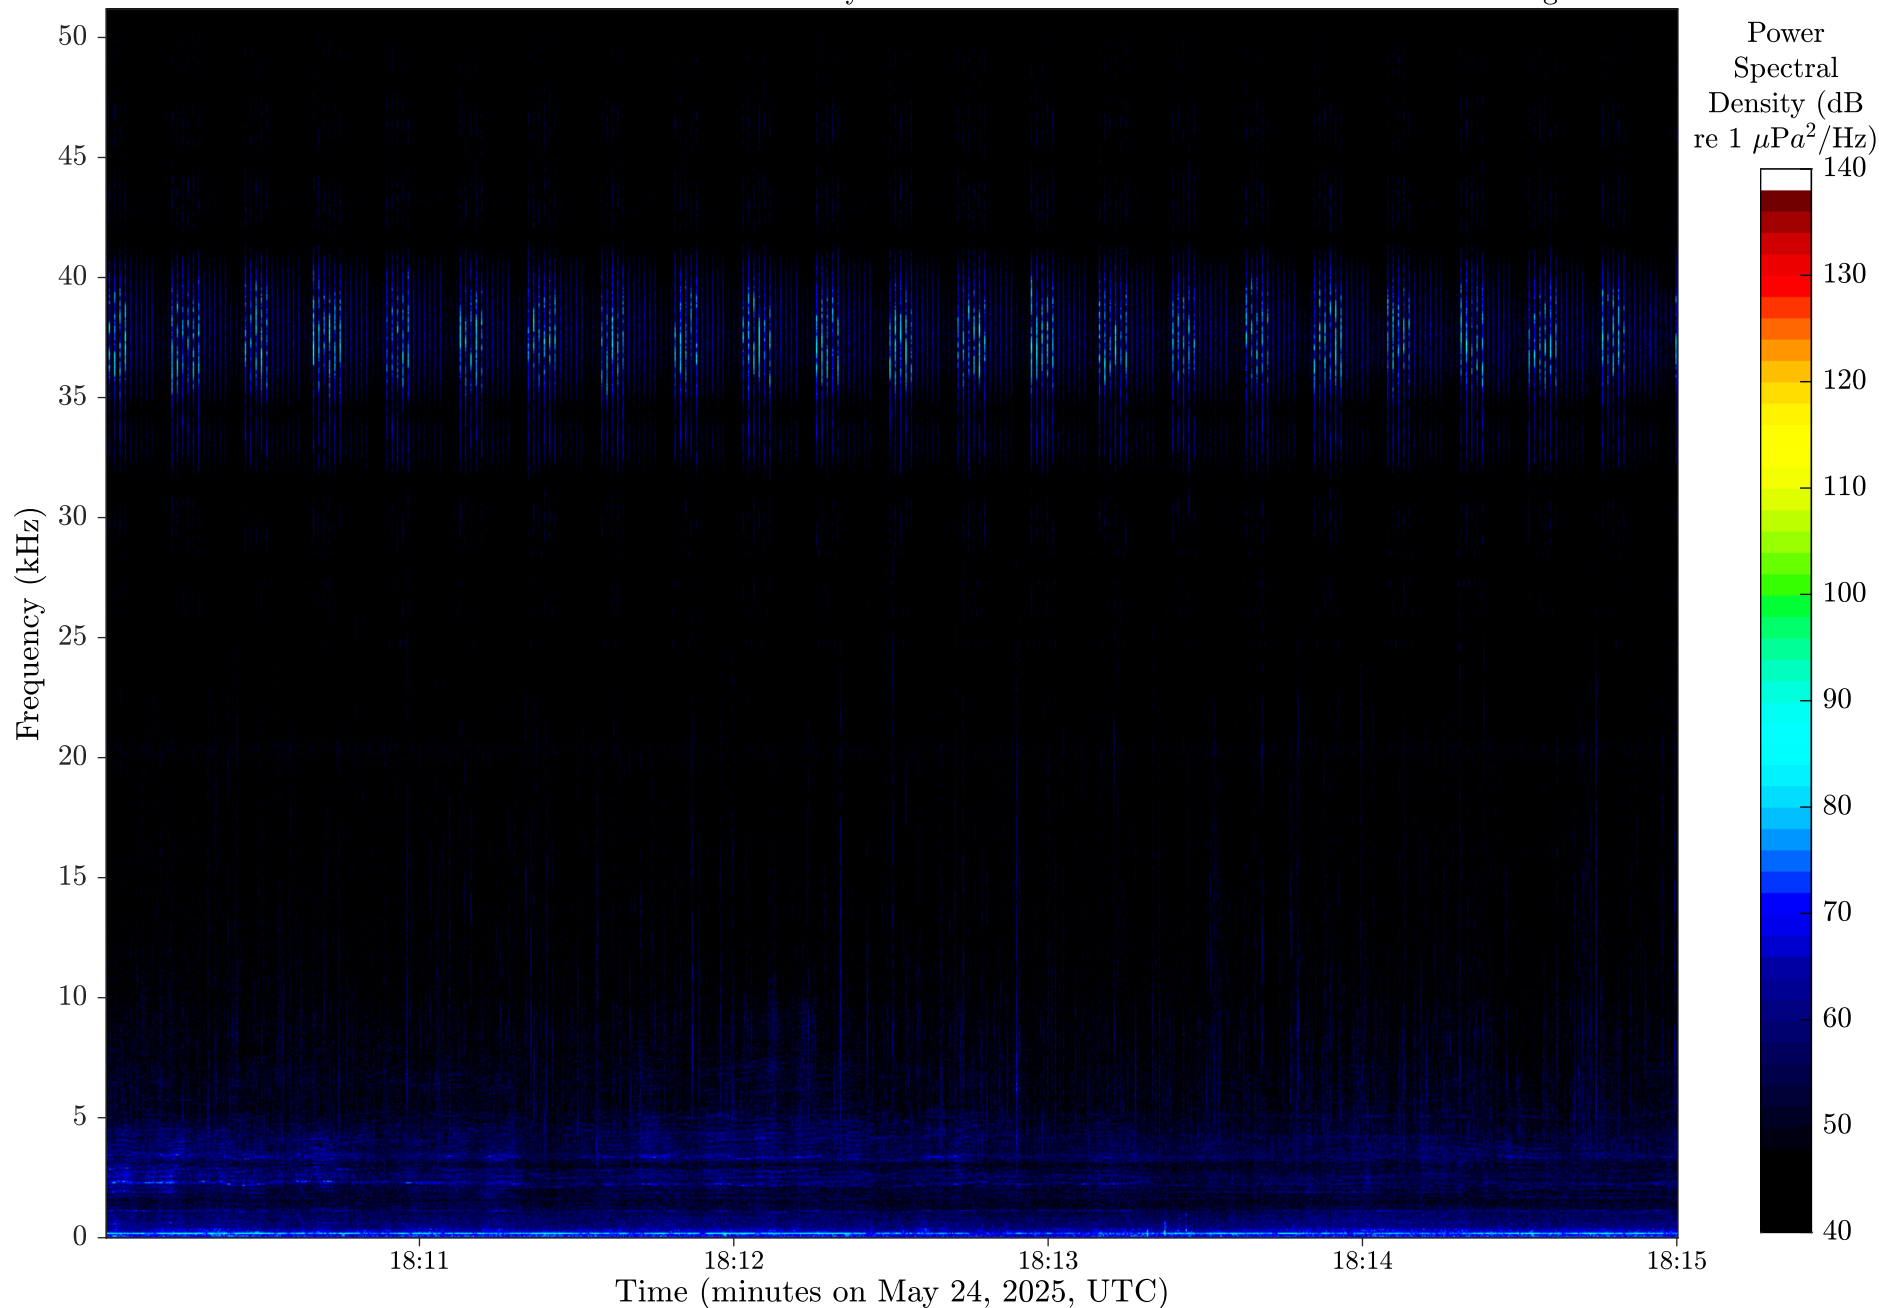


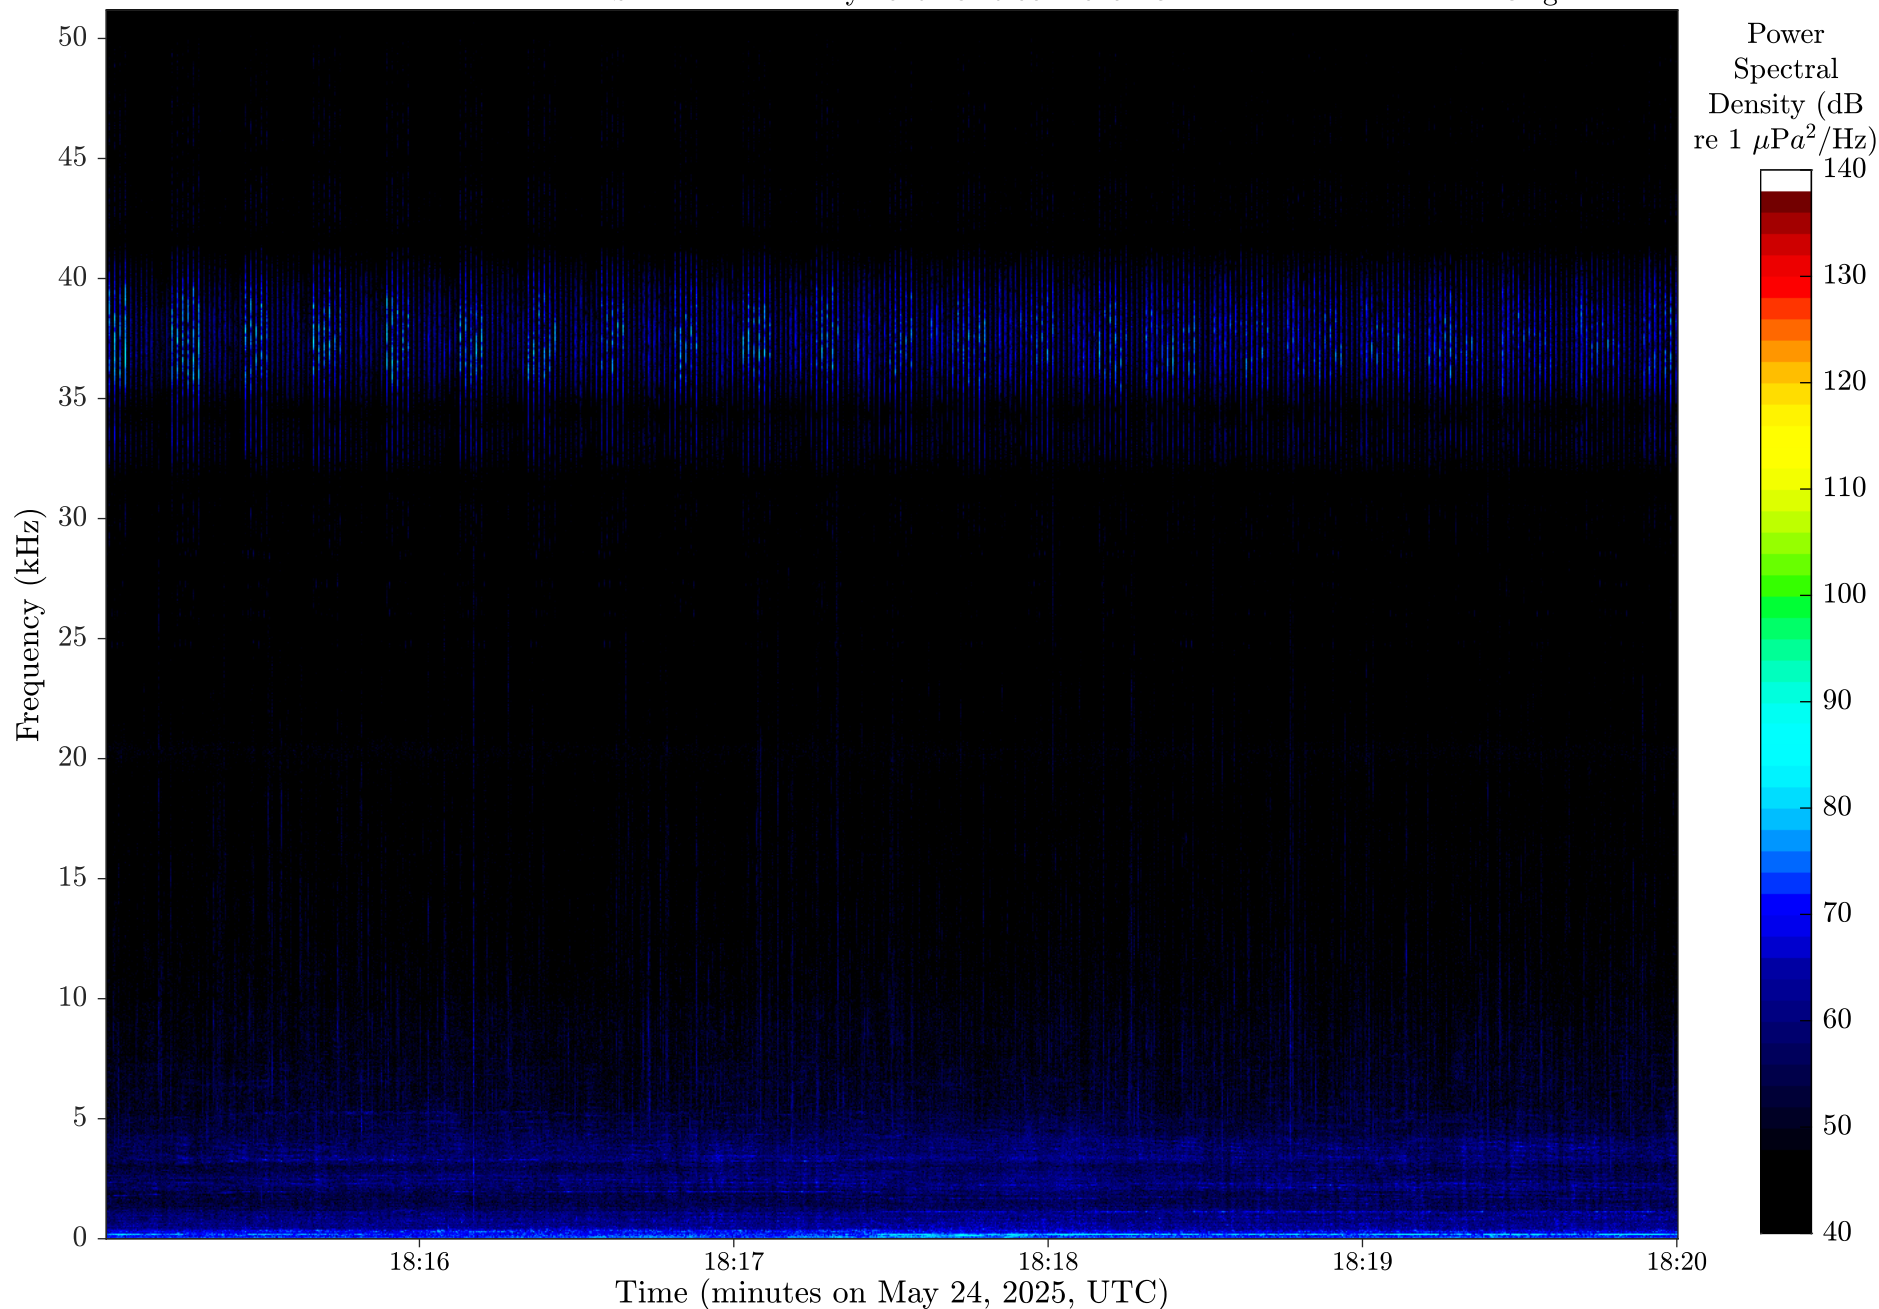

Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:48:47 UTC

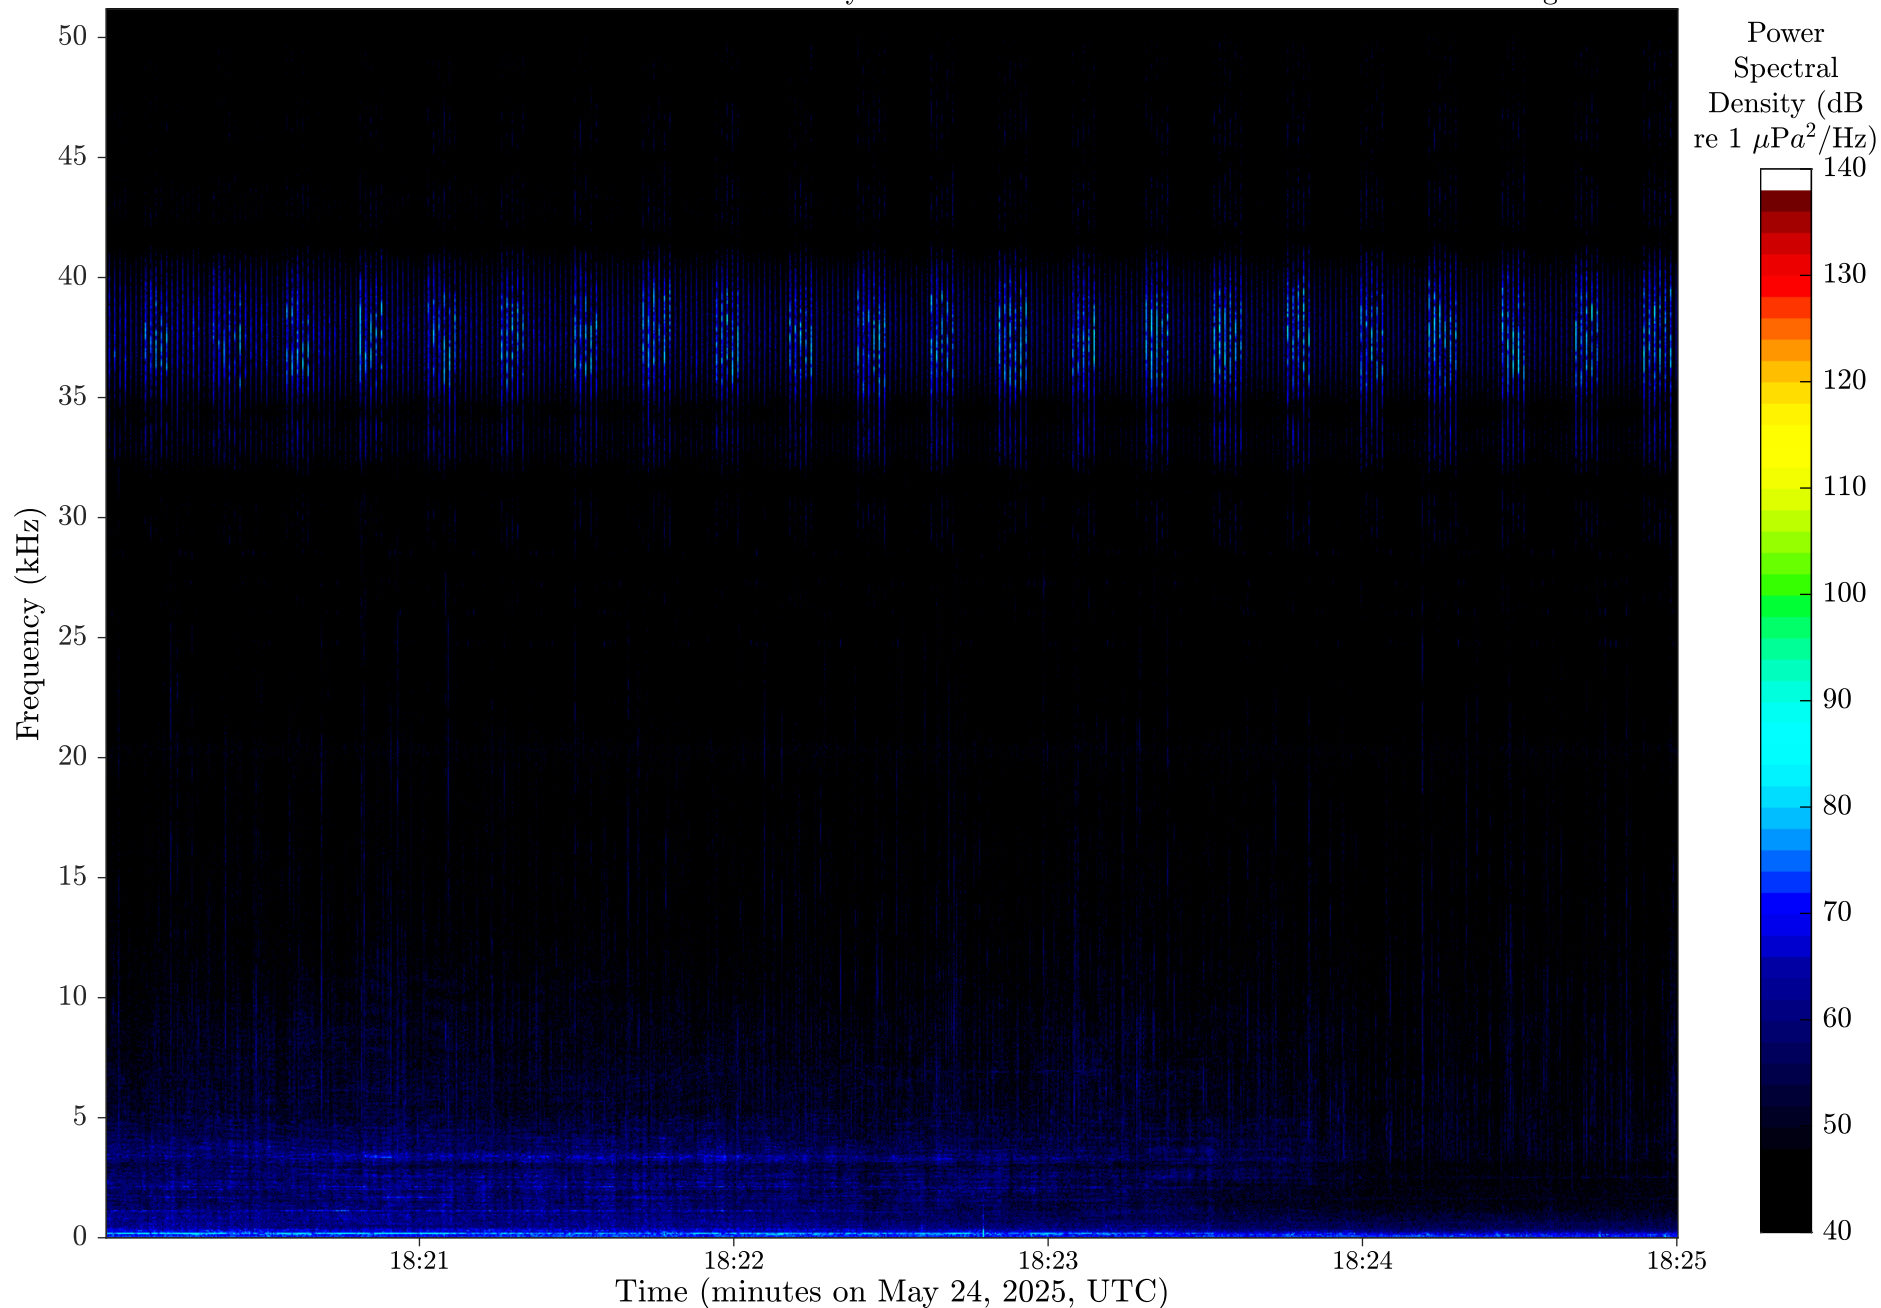

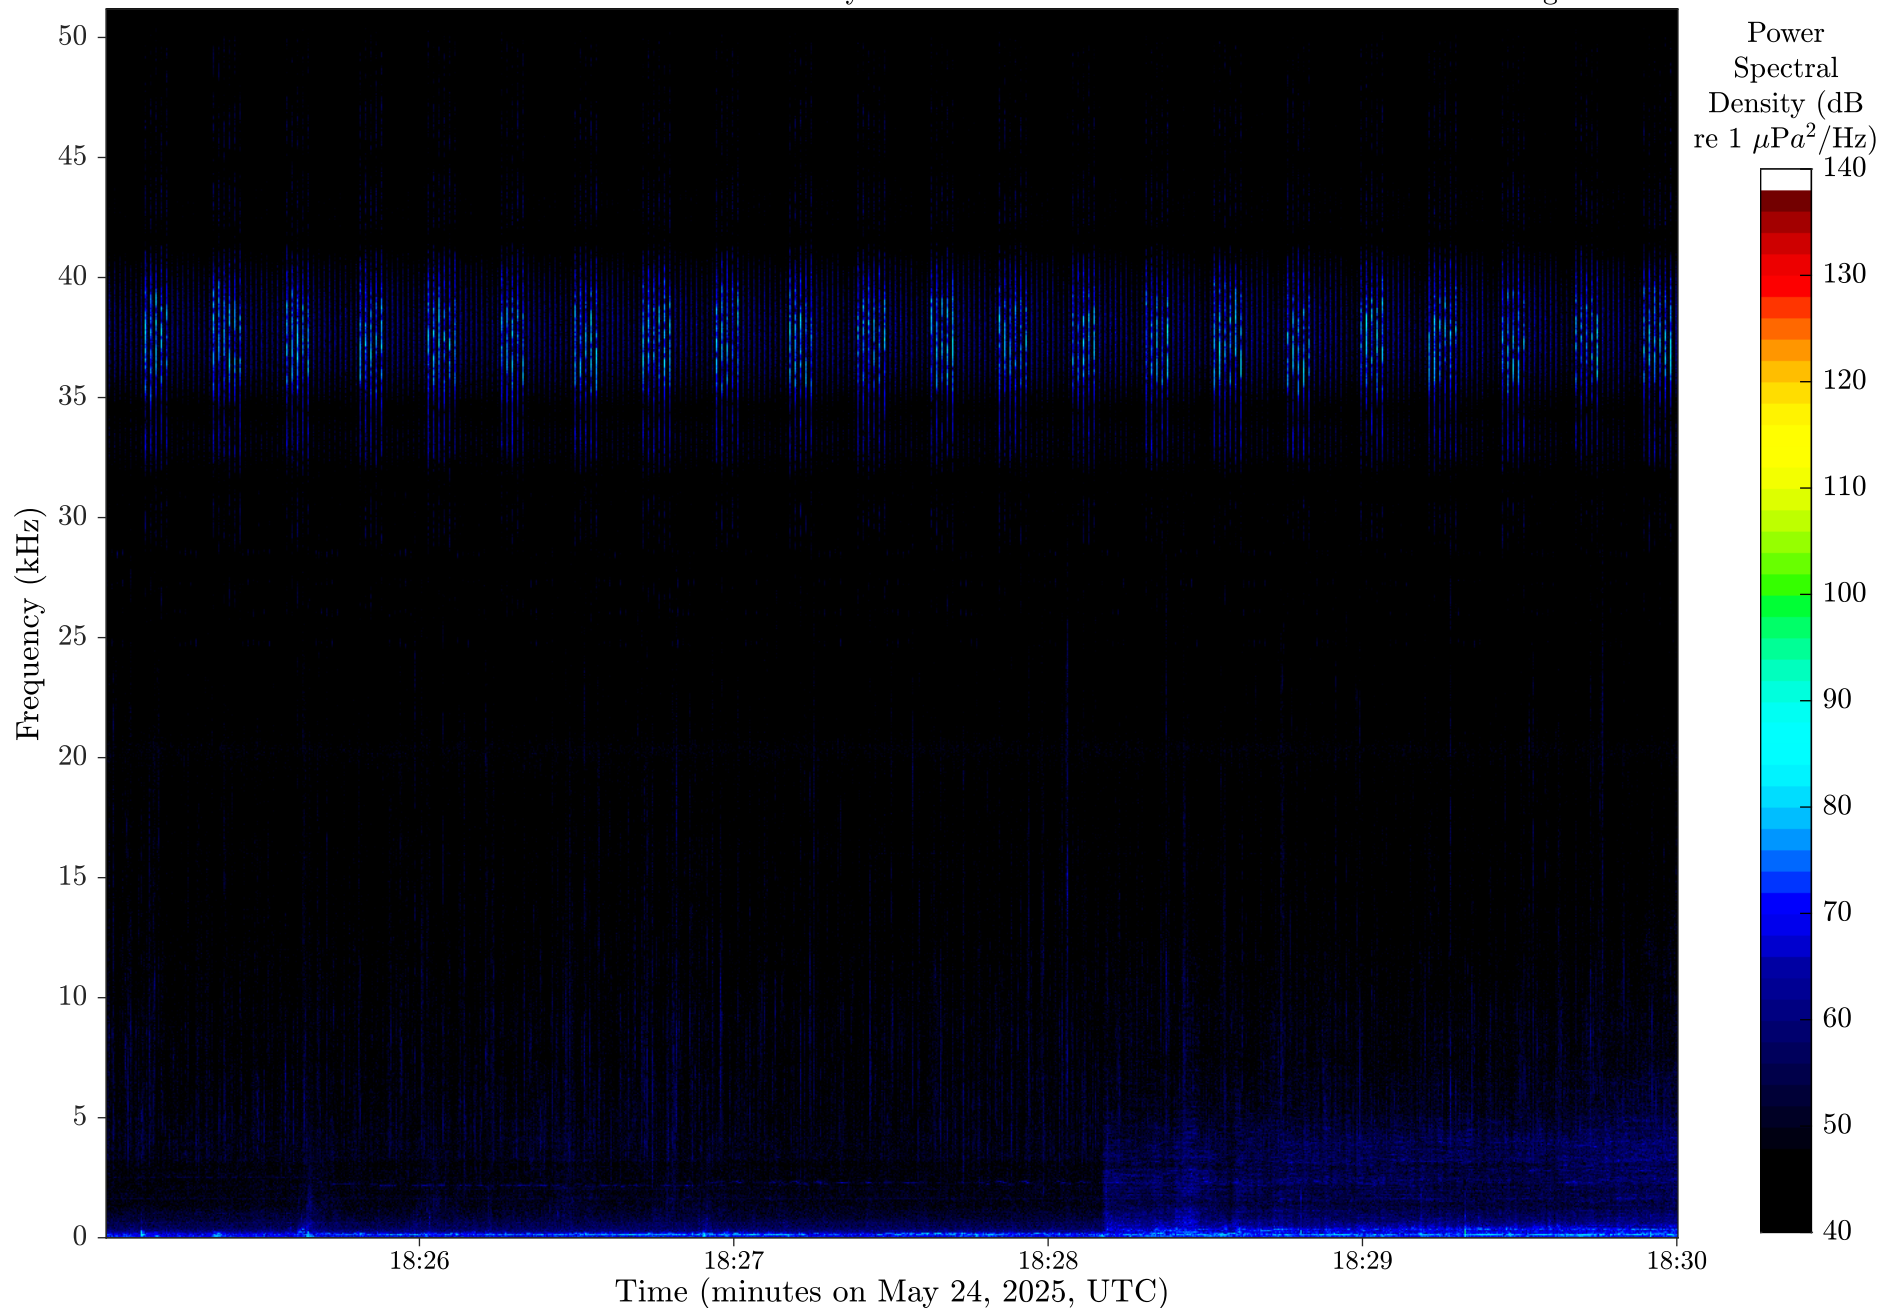


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:04 UTC

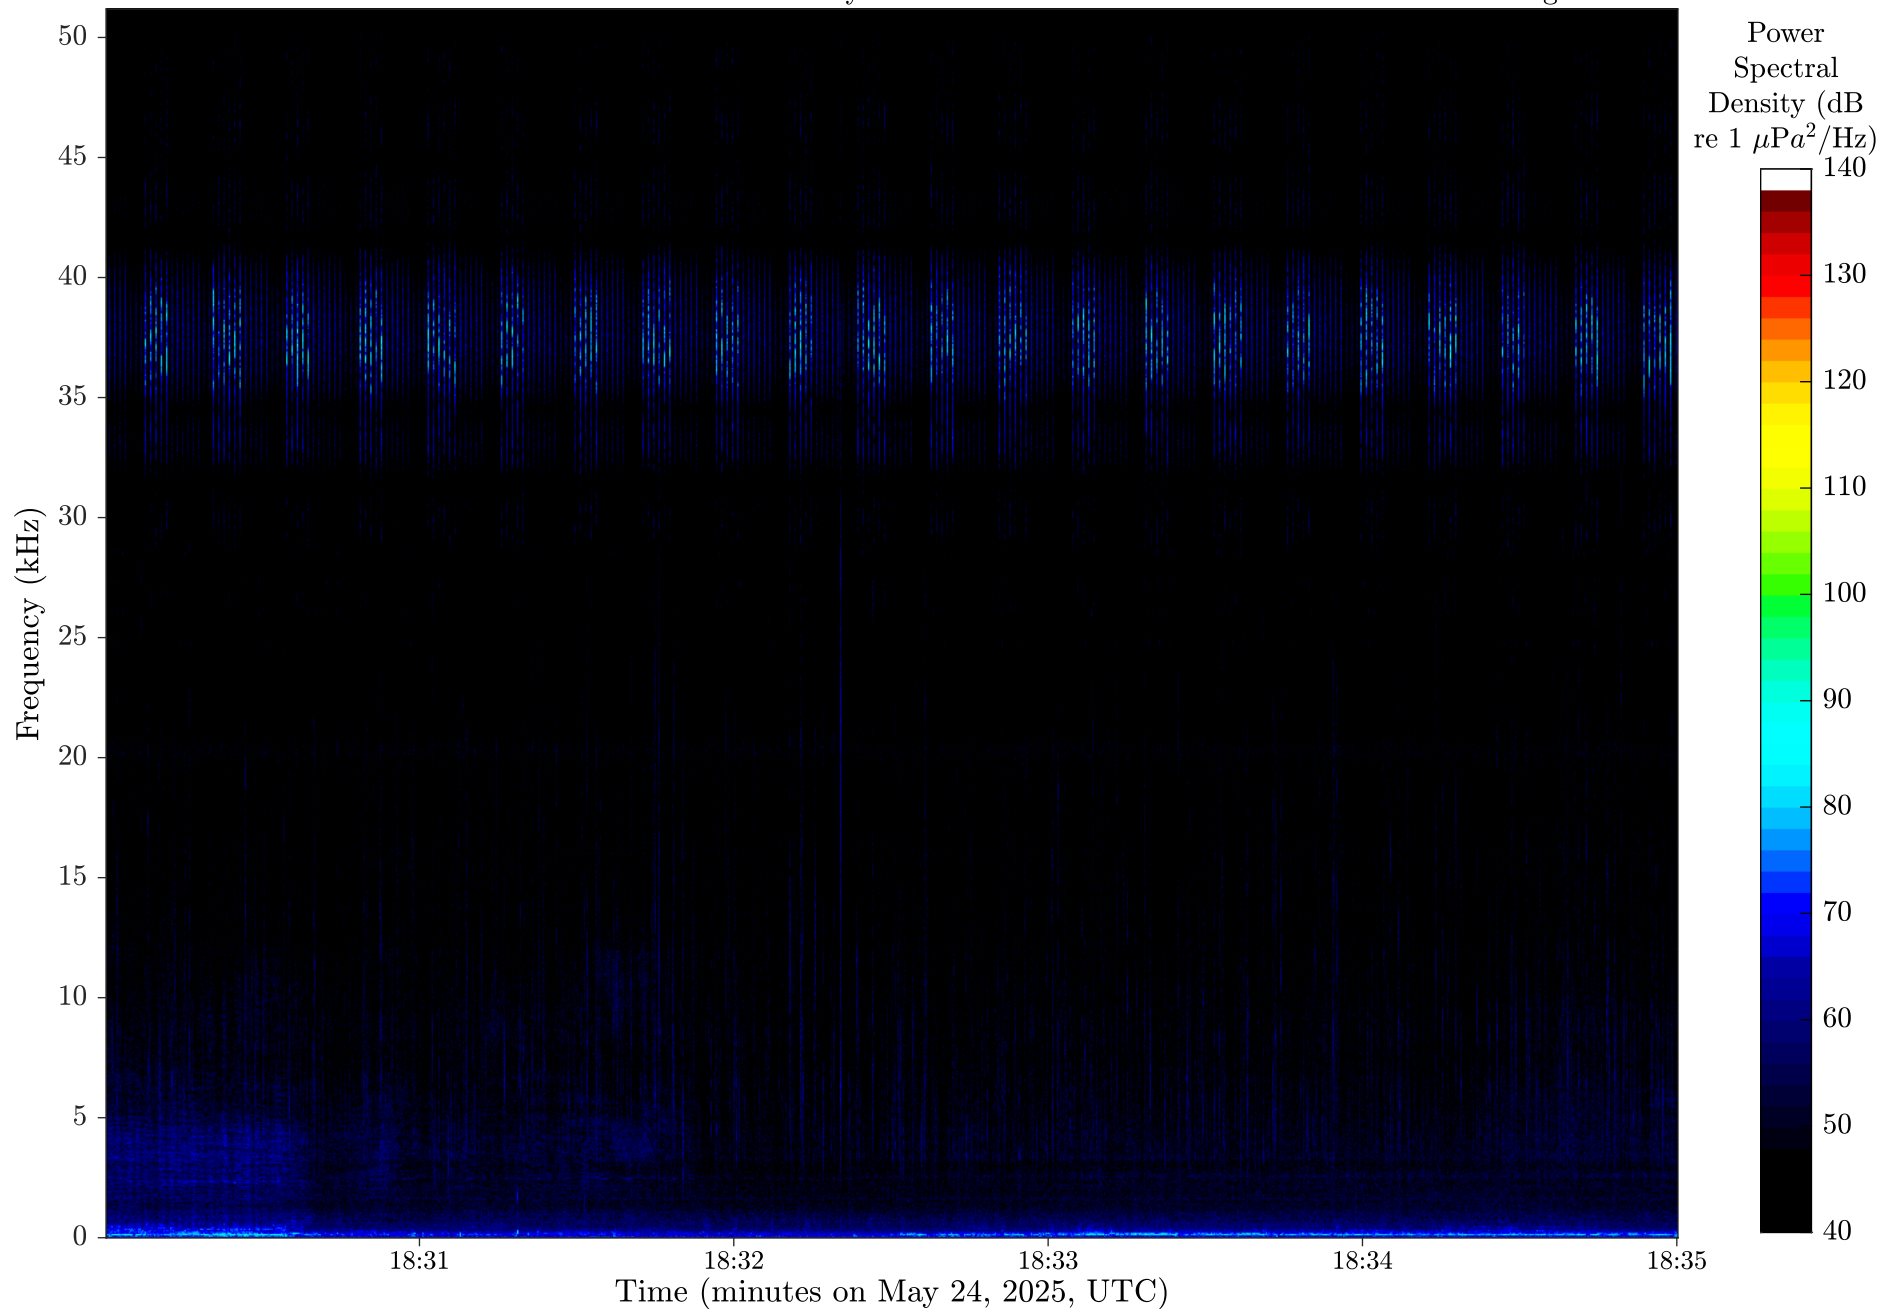


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:11 UTC

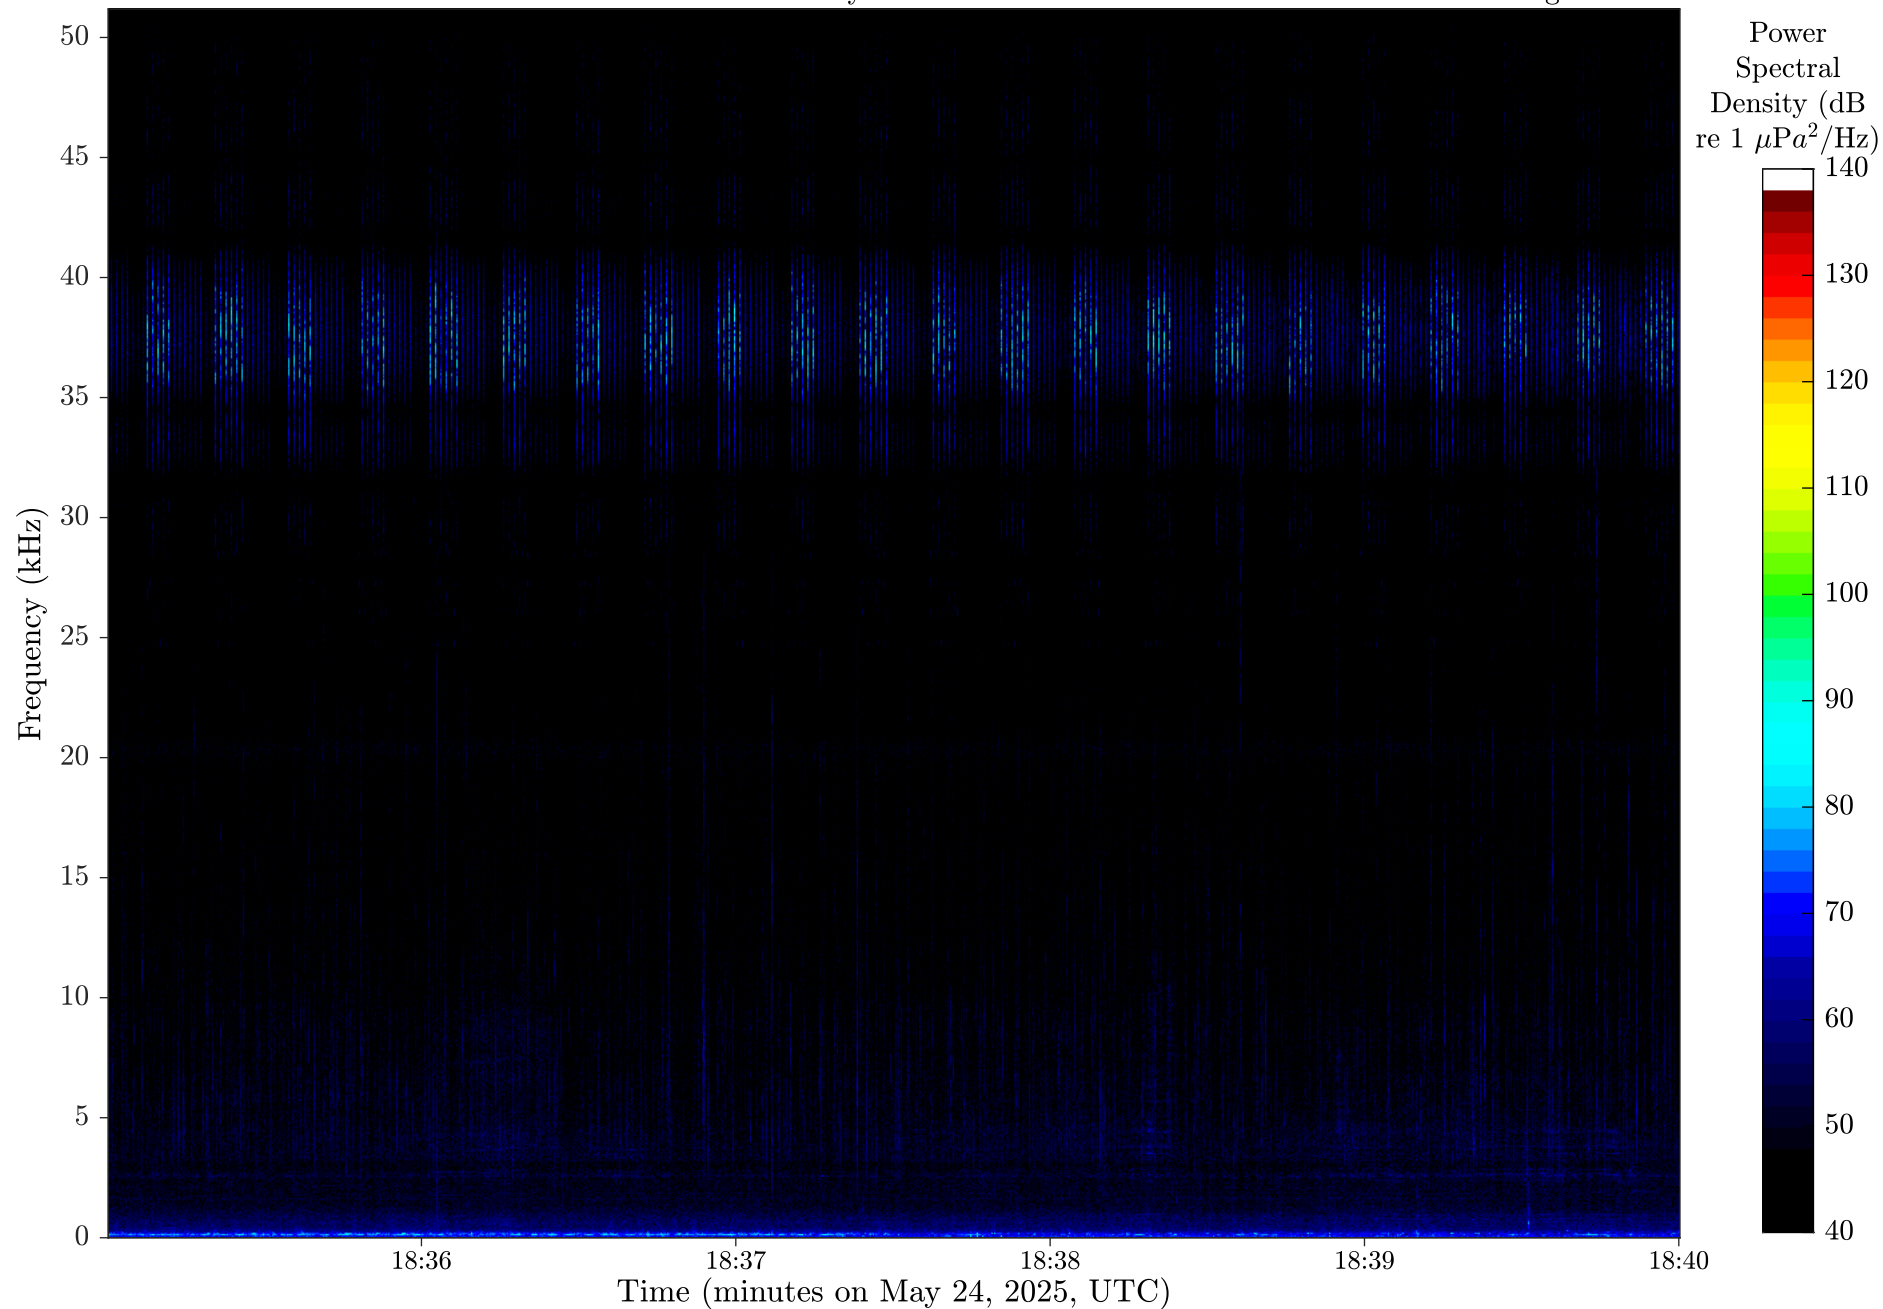


Comments: 31.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:19 UTC

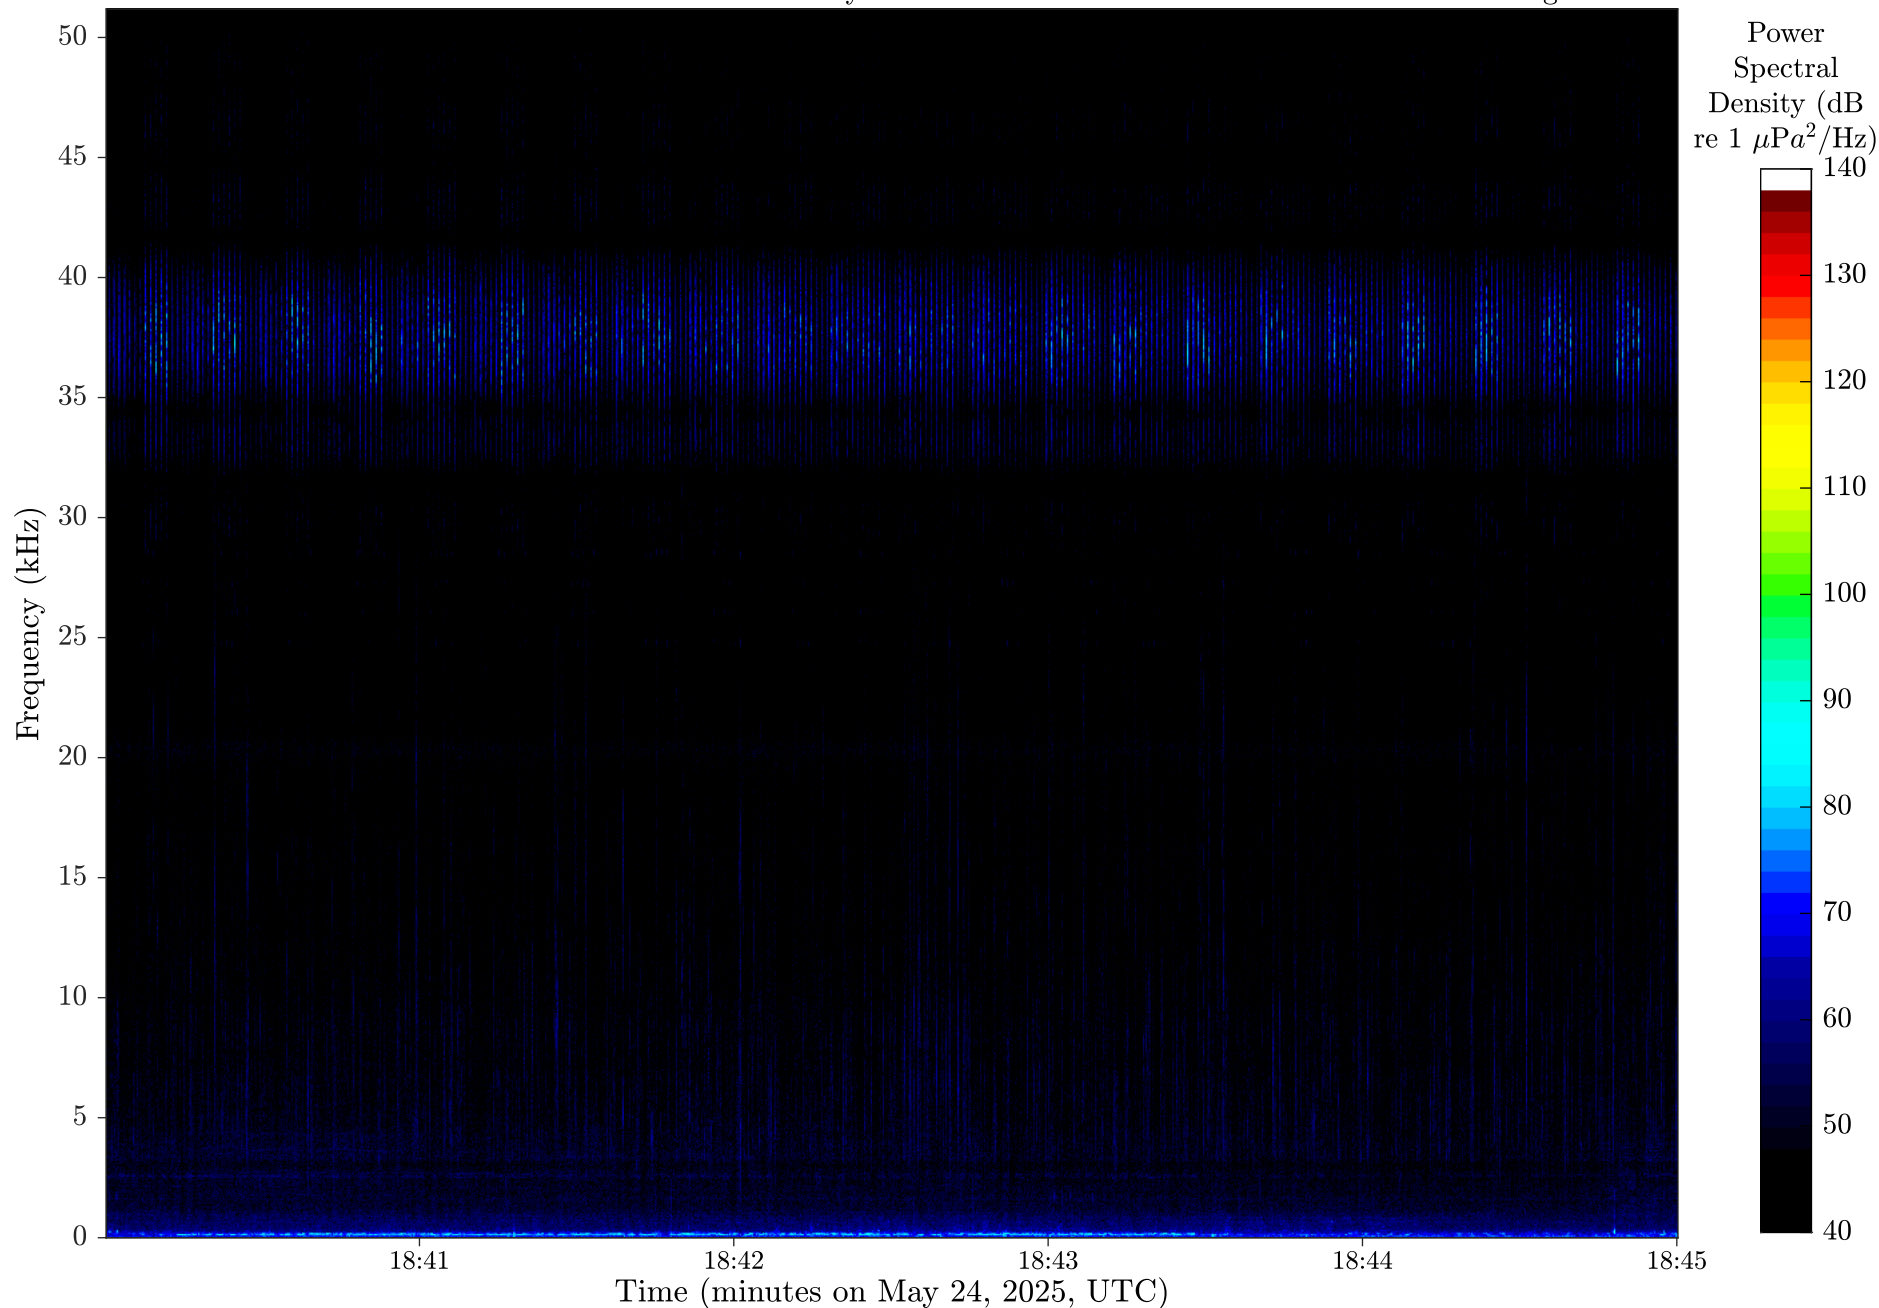


Comments: 30.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:27 UTC

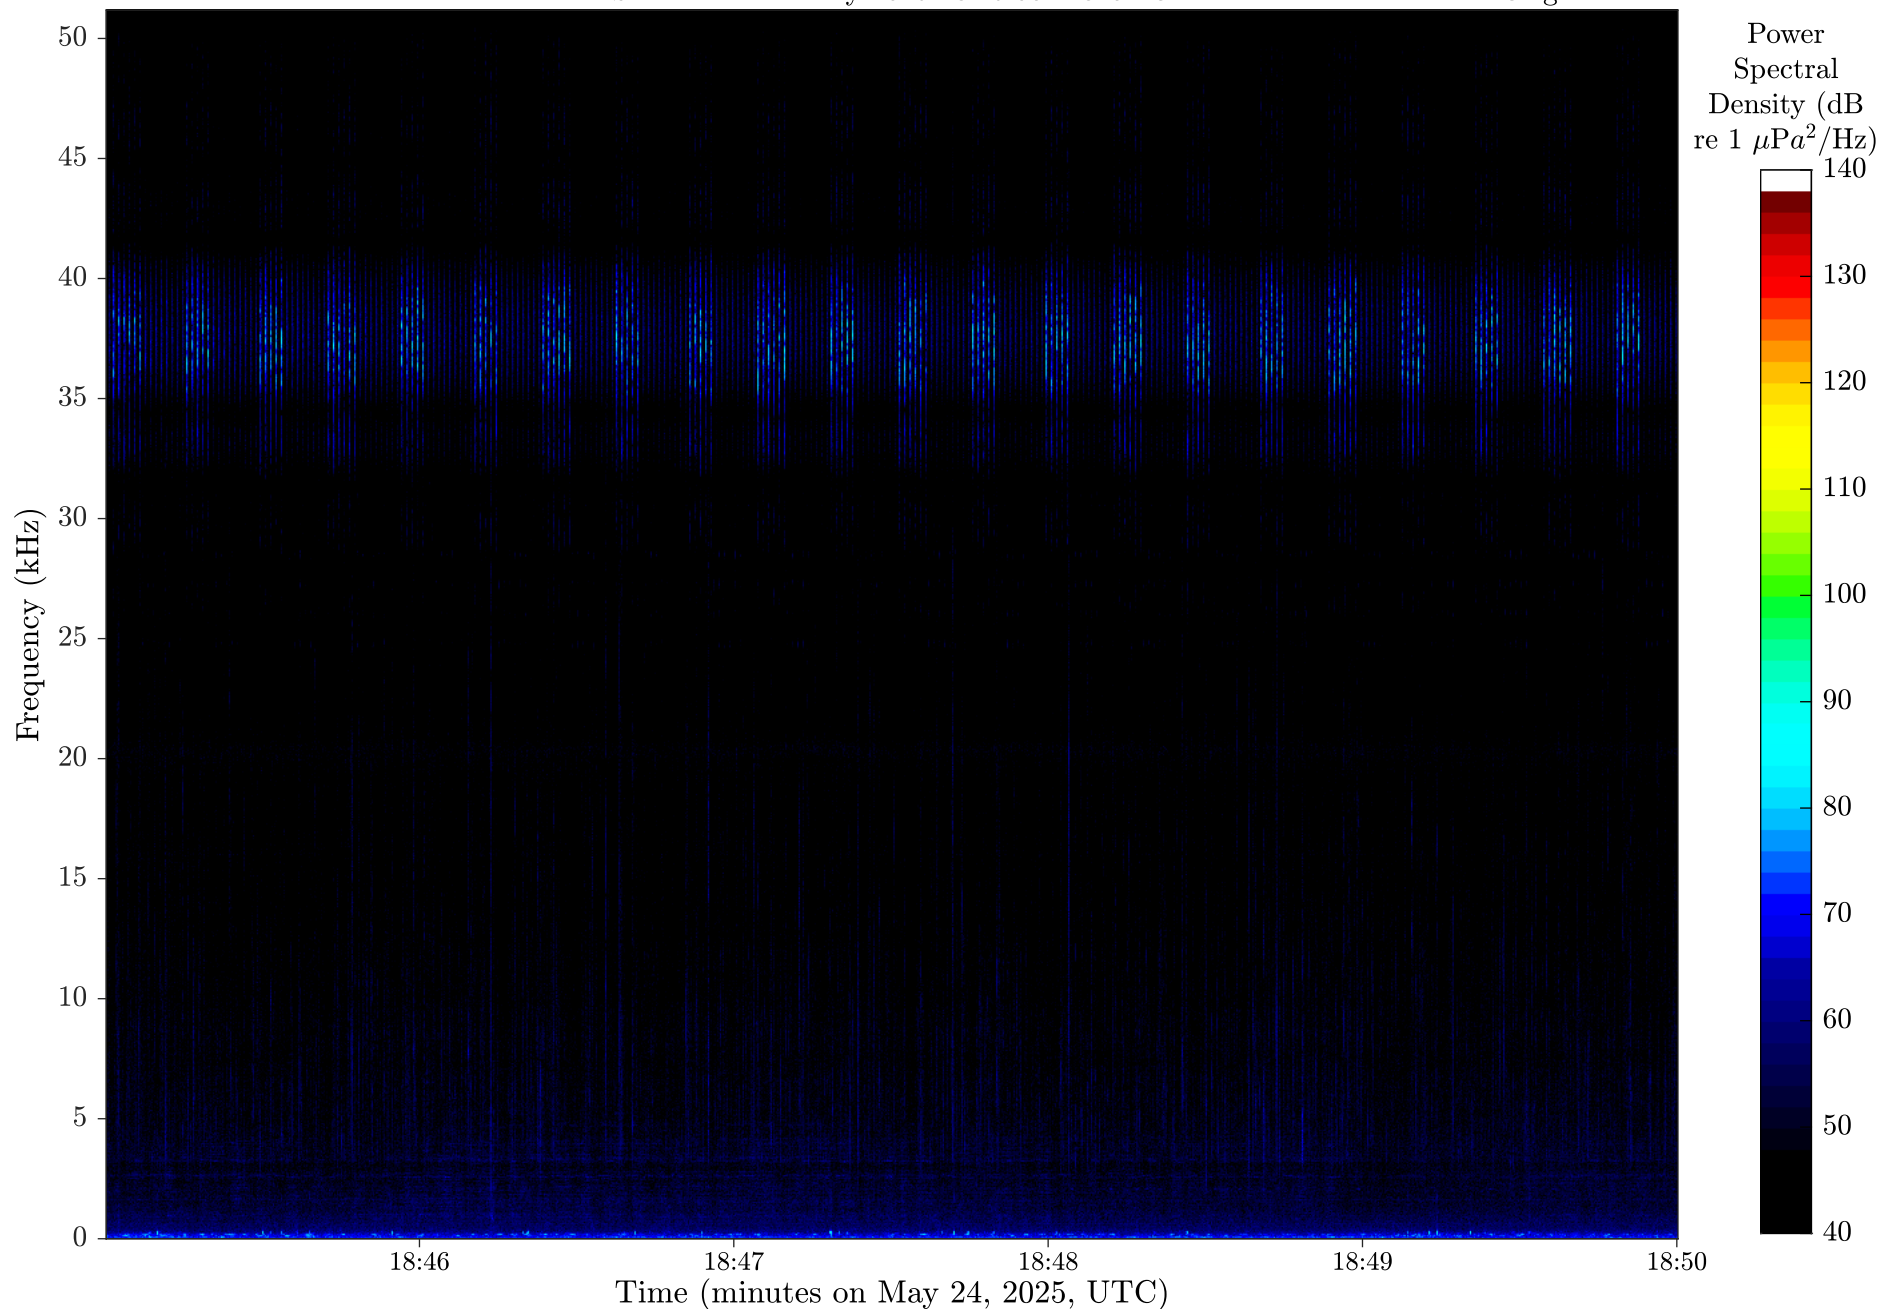


Comments: 31.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:35 UTC

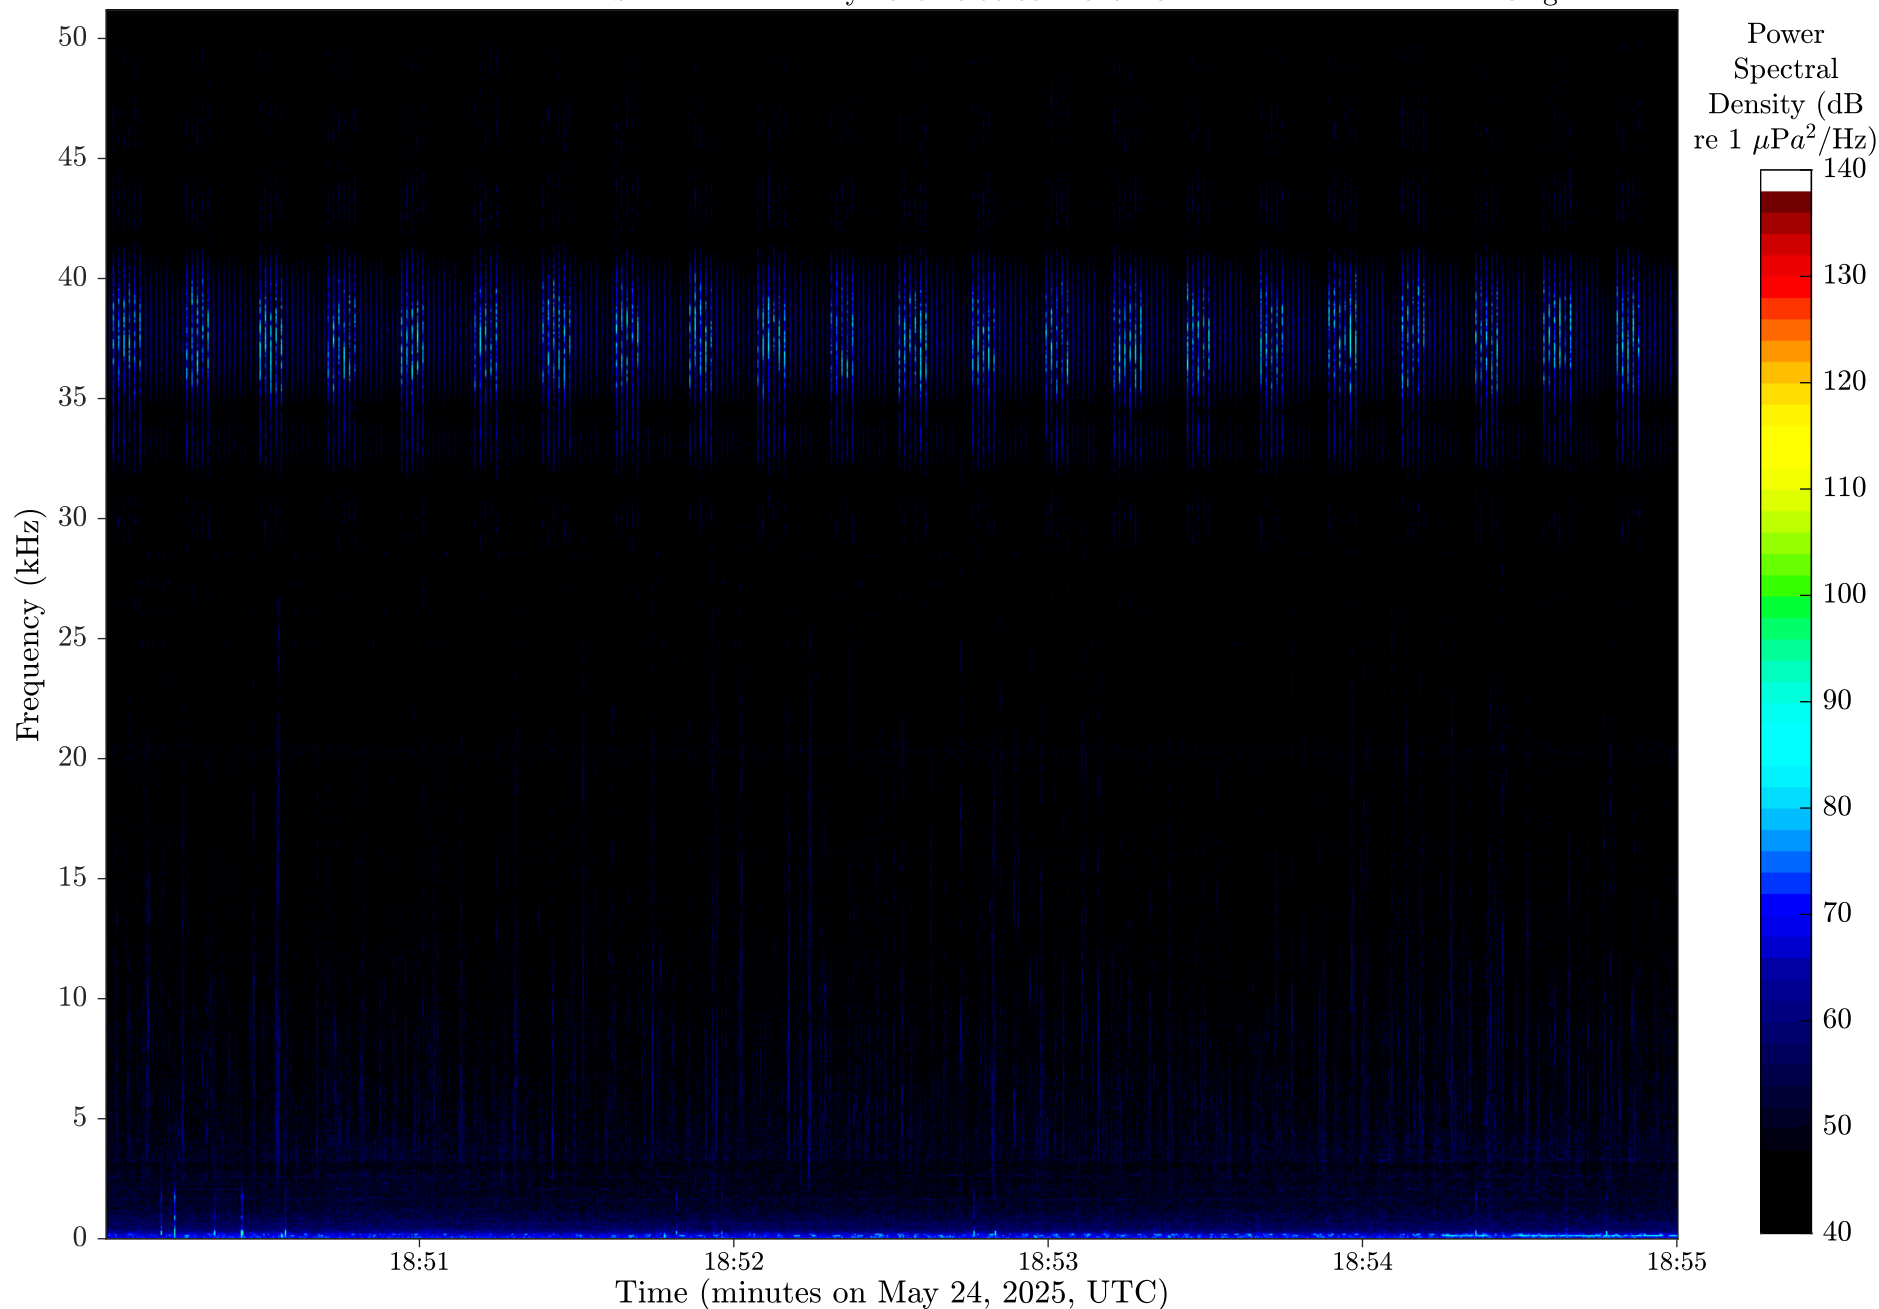


Comments: 32.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:44 UTC

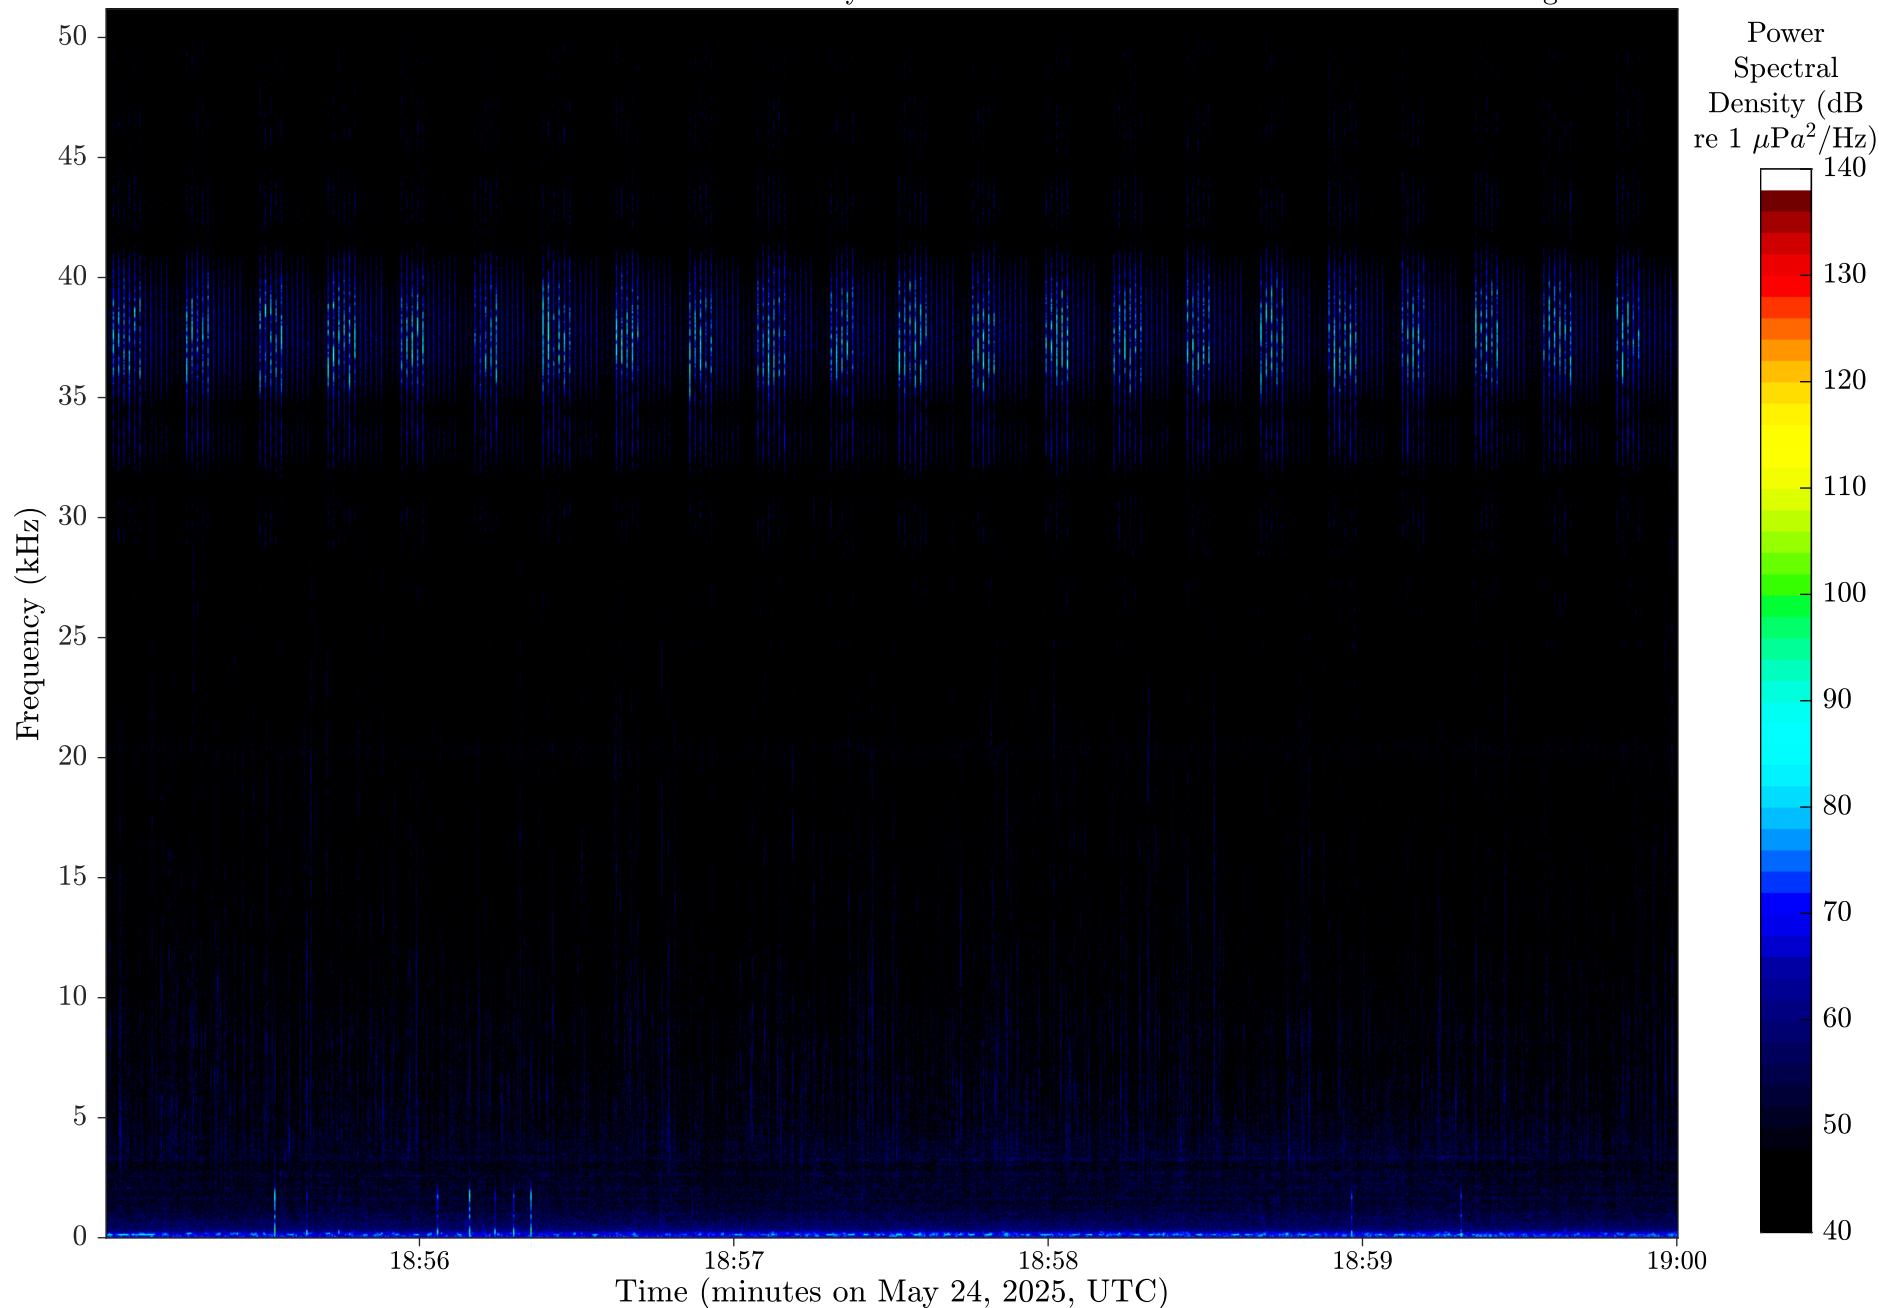


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:49:52 UTC

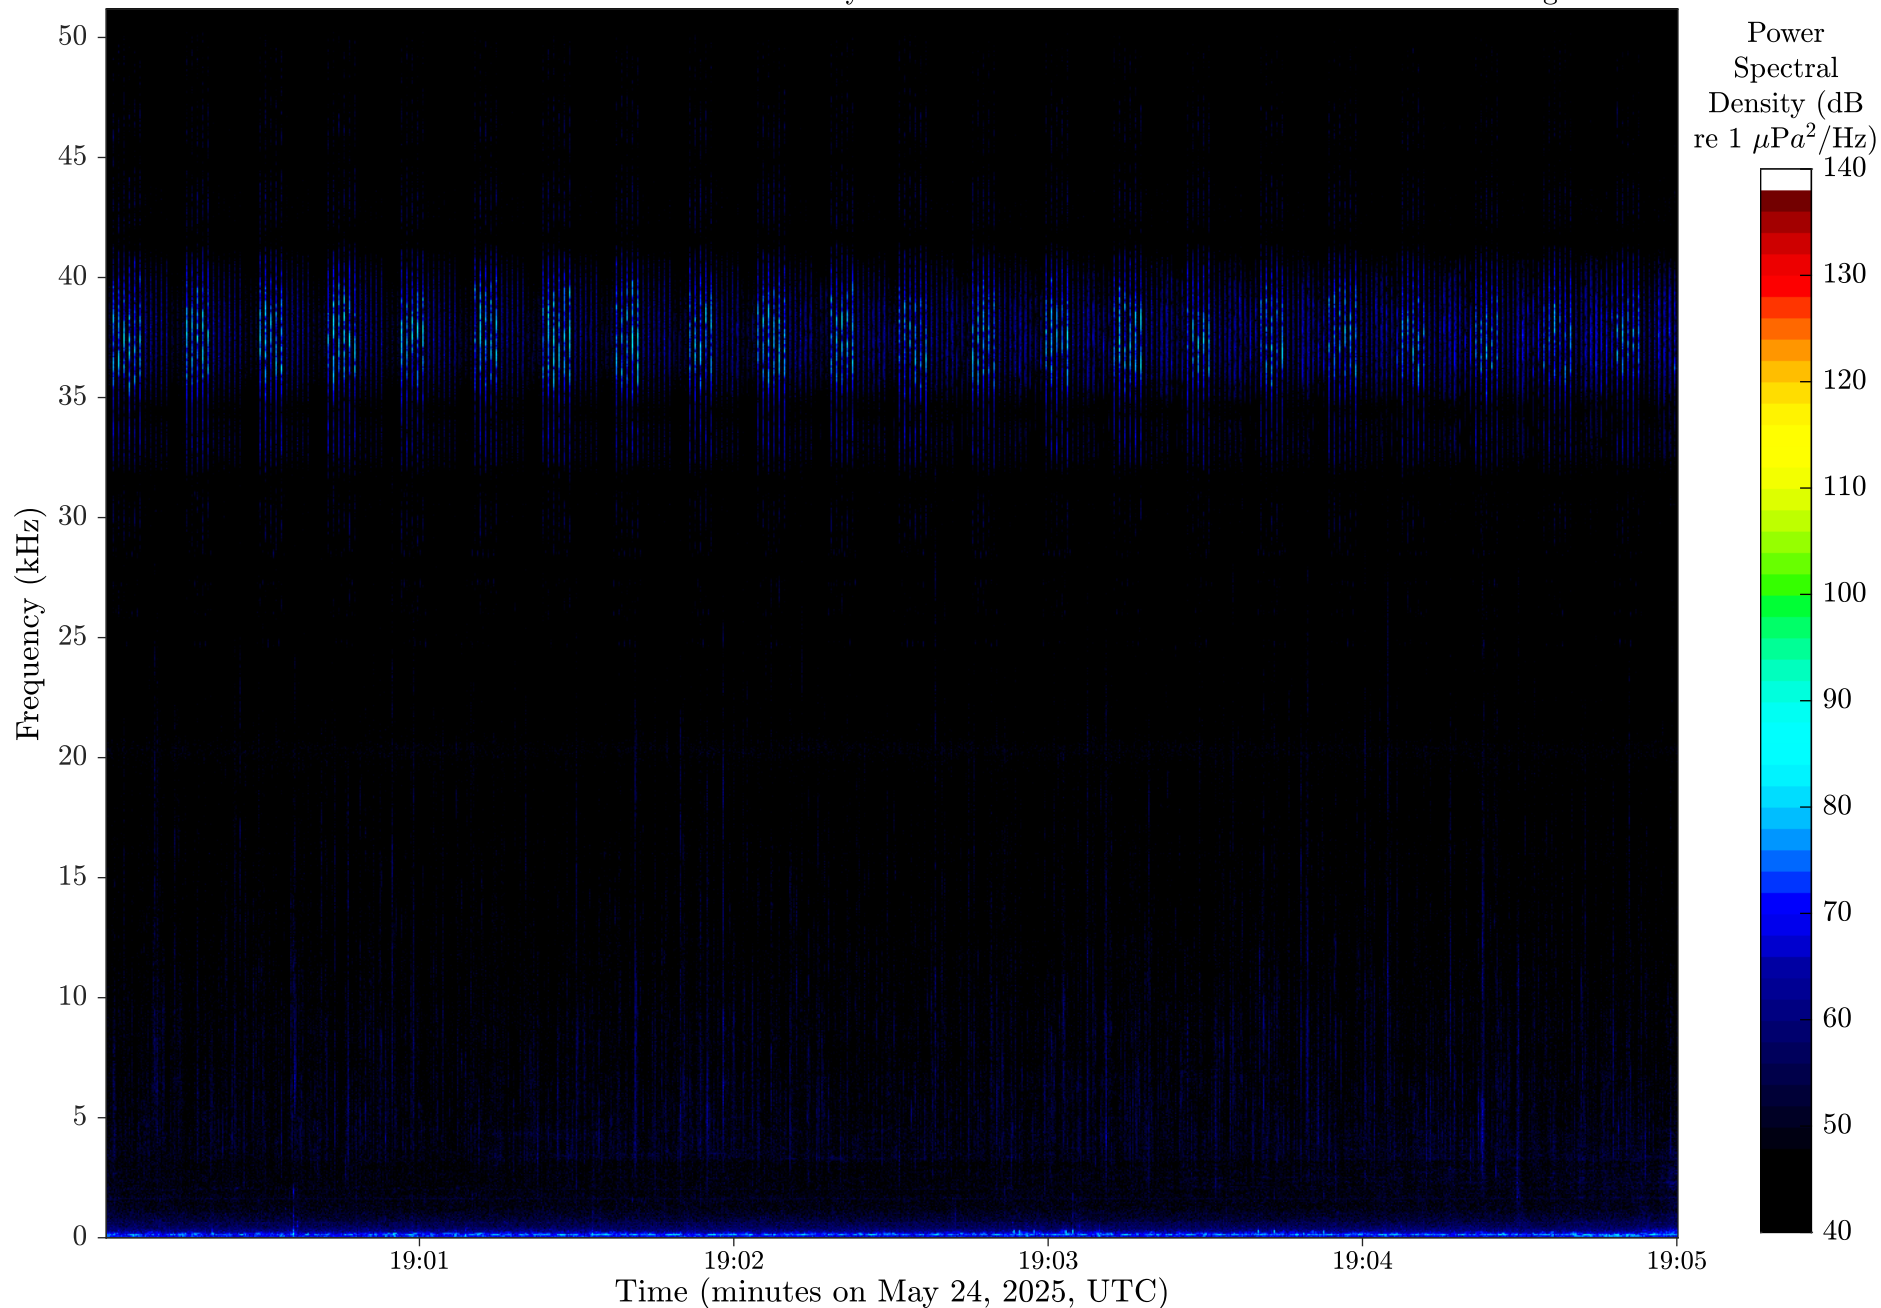


Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:49:59 UTC

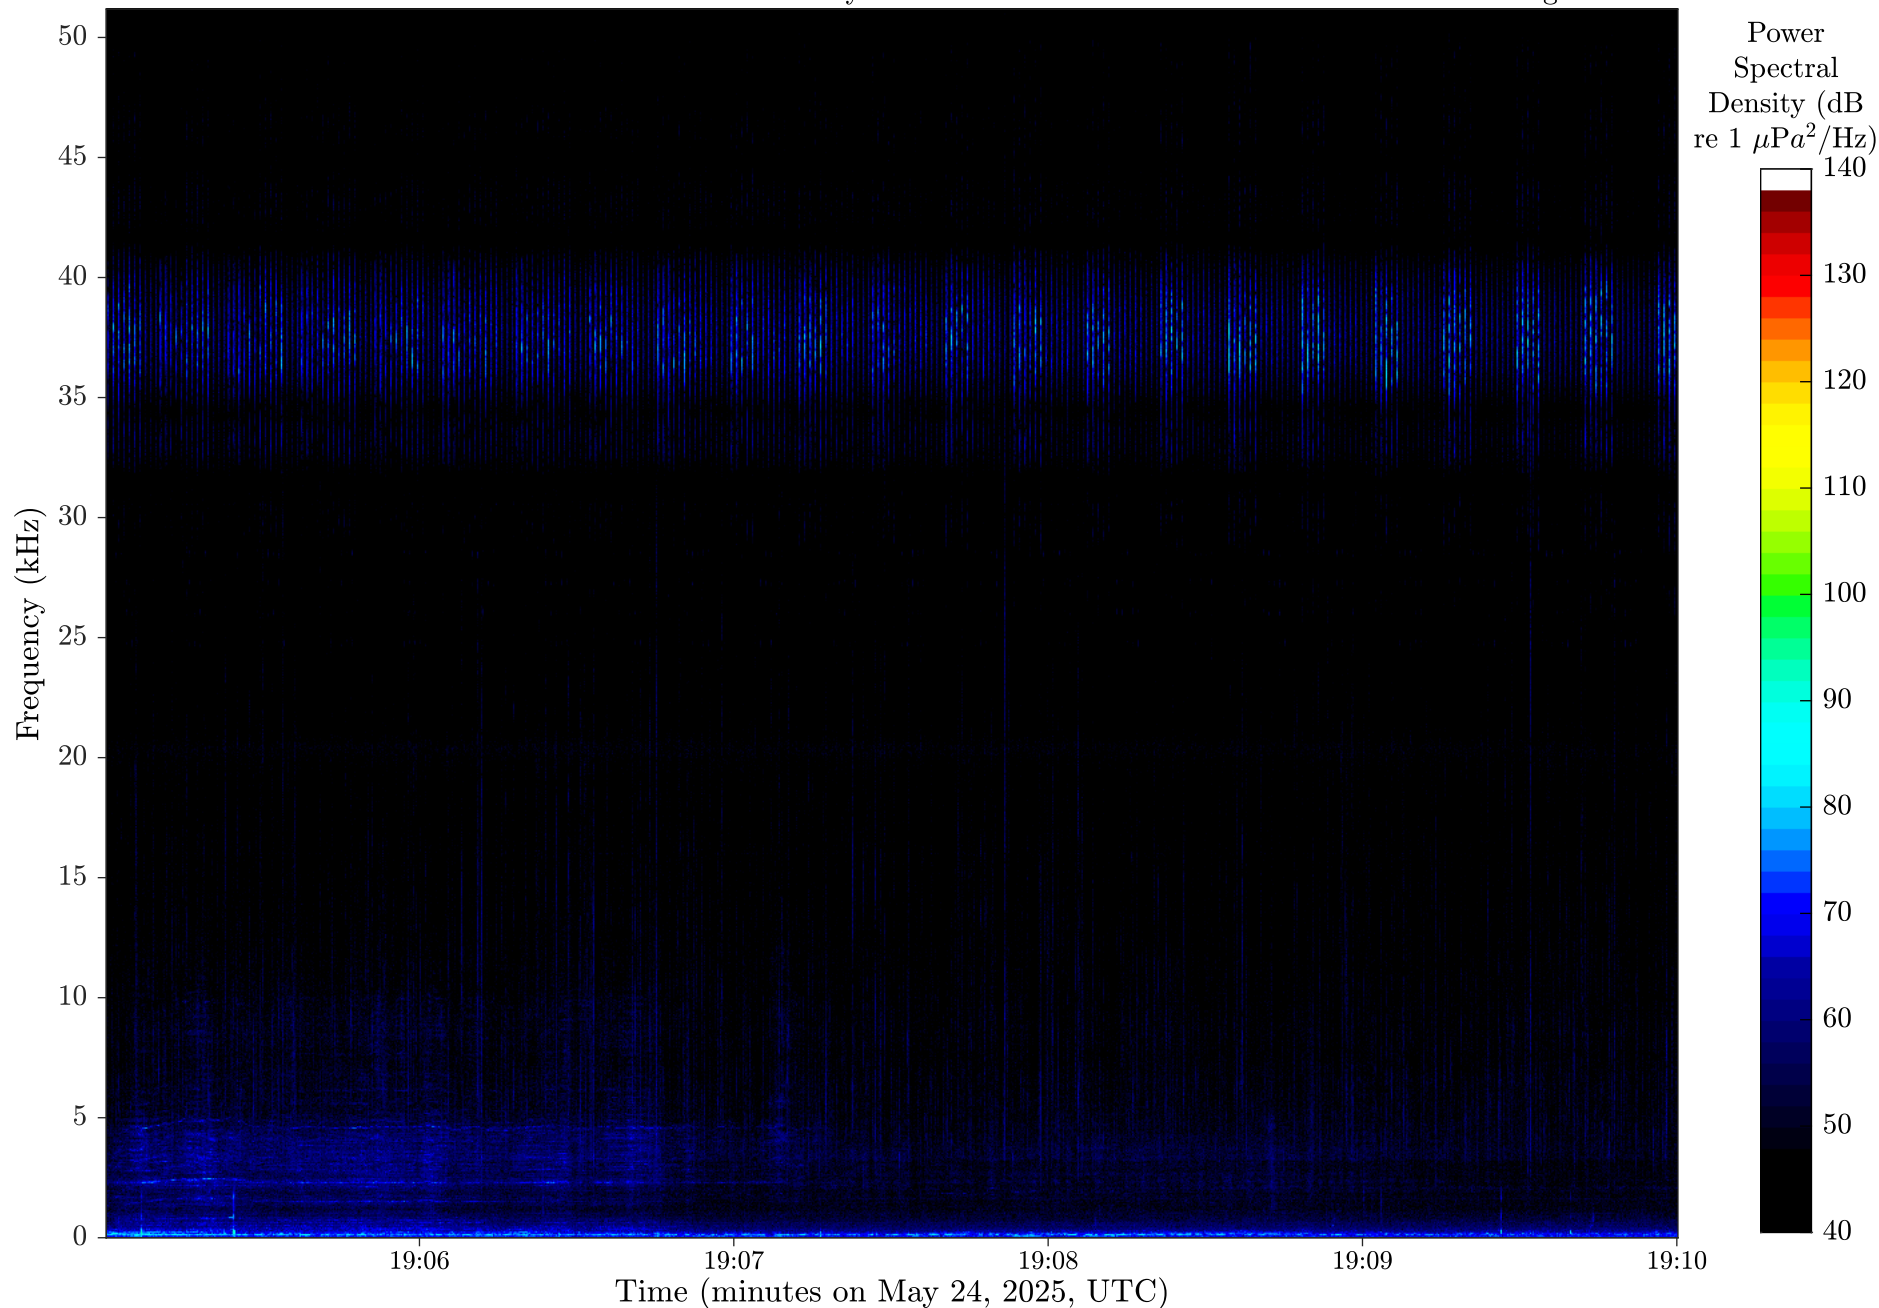

Comments: 32.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:50:08 UTC

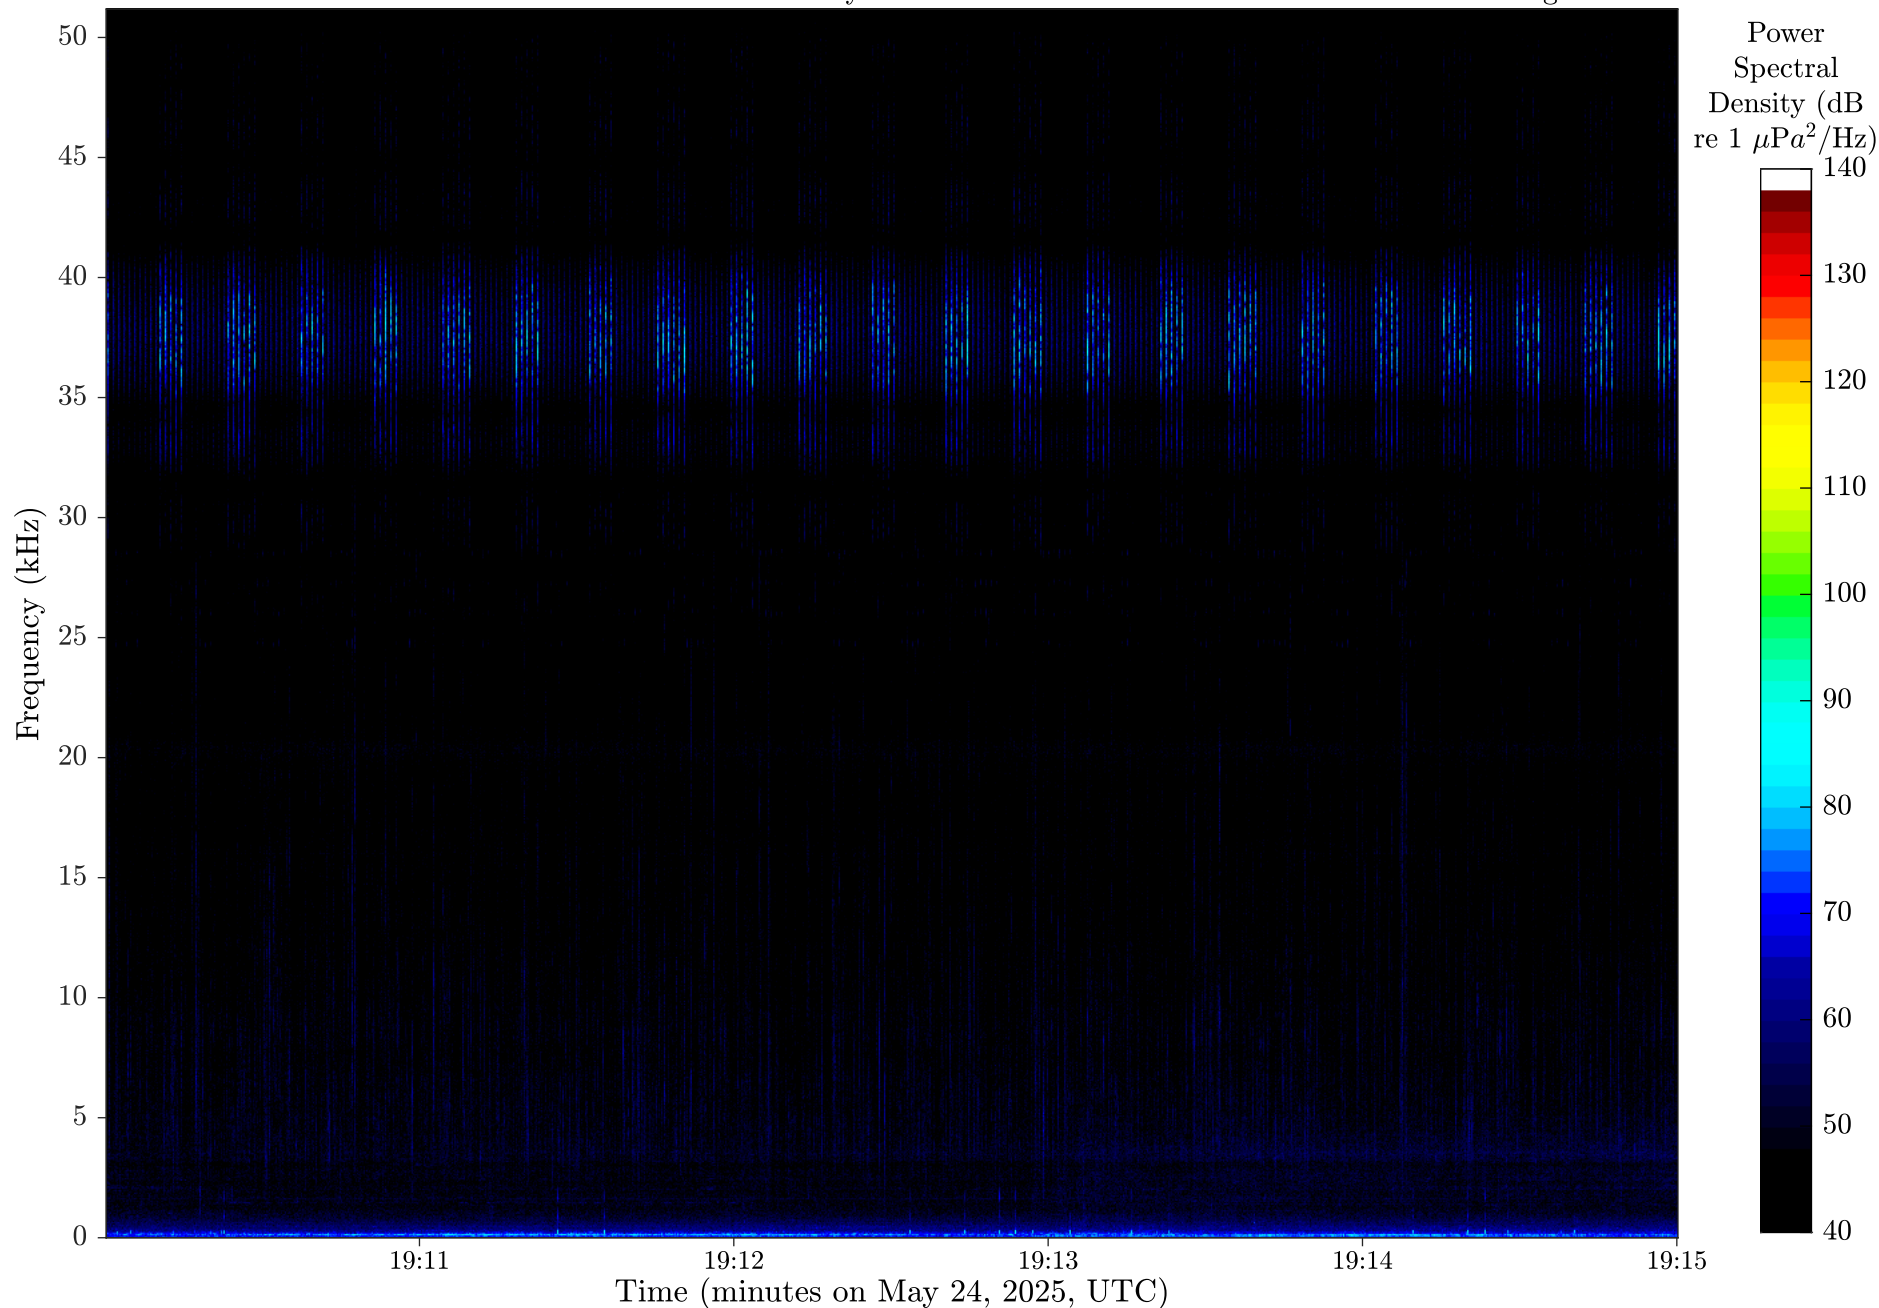

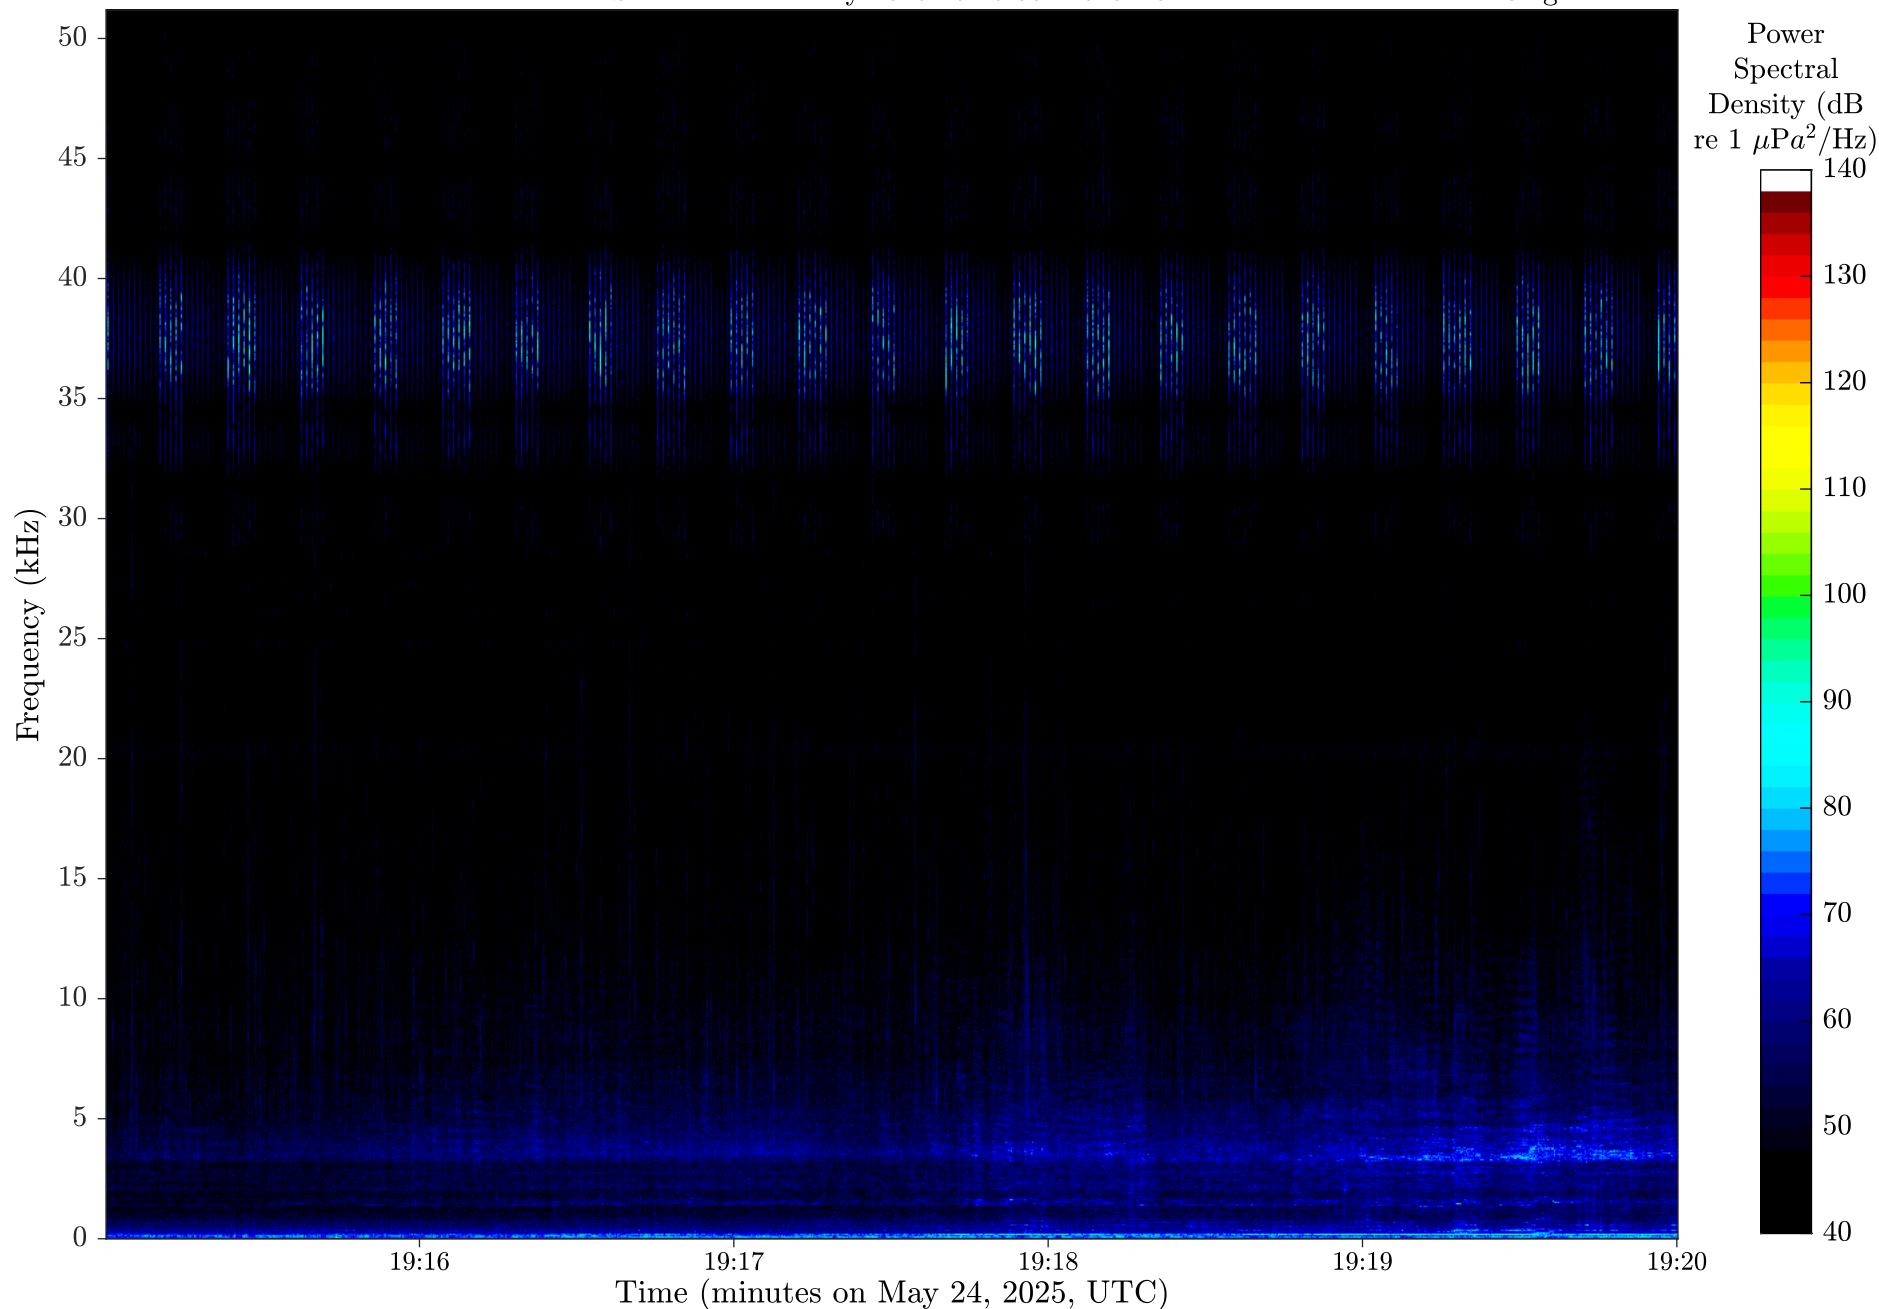


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:50:24 UTC

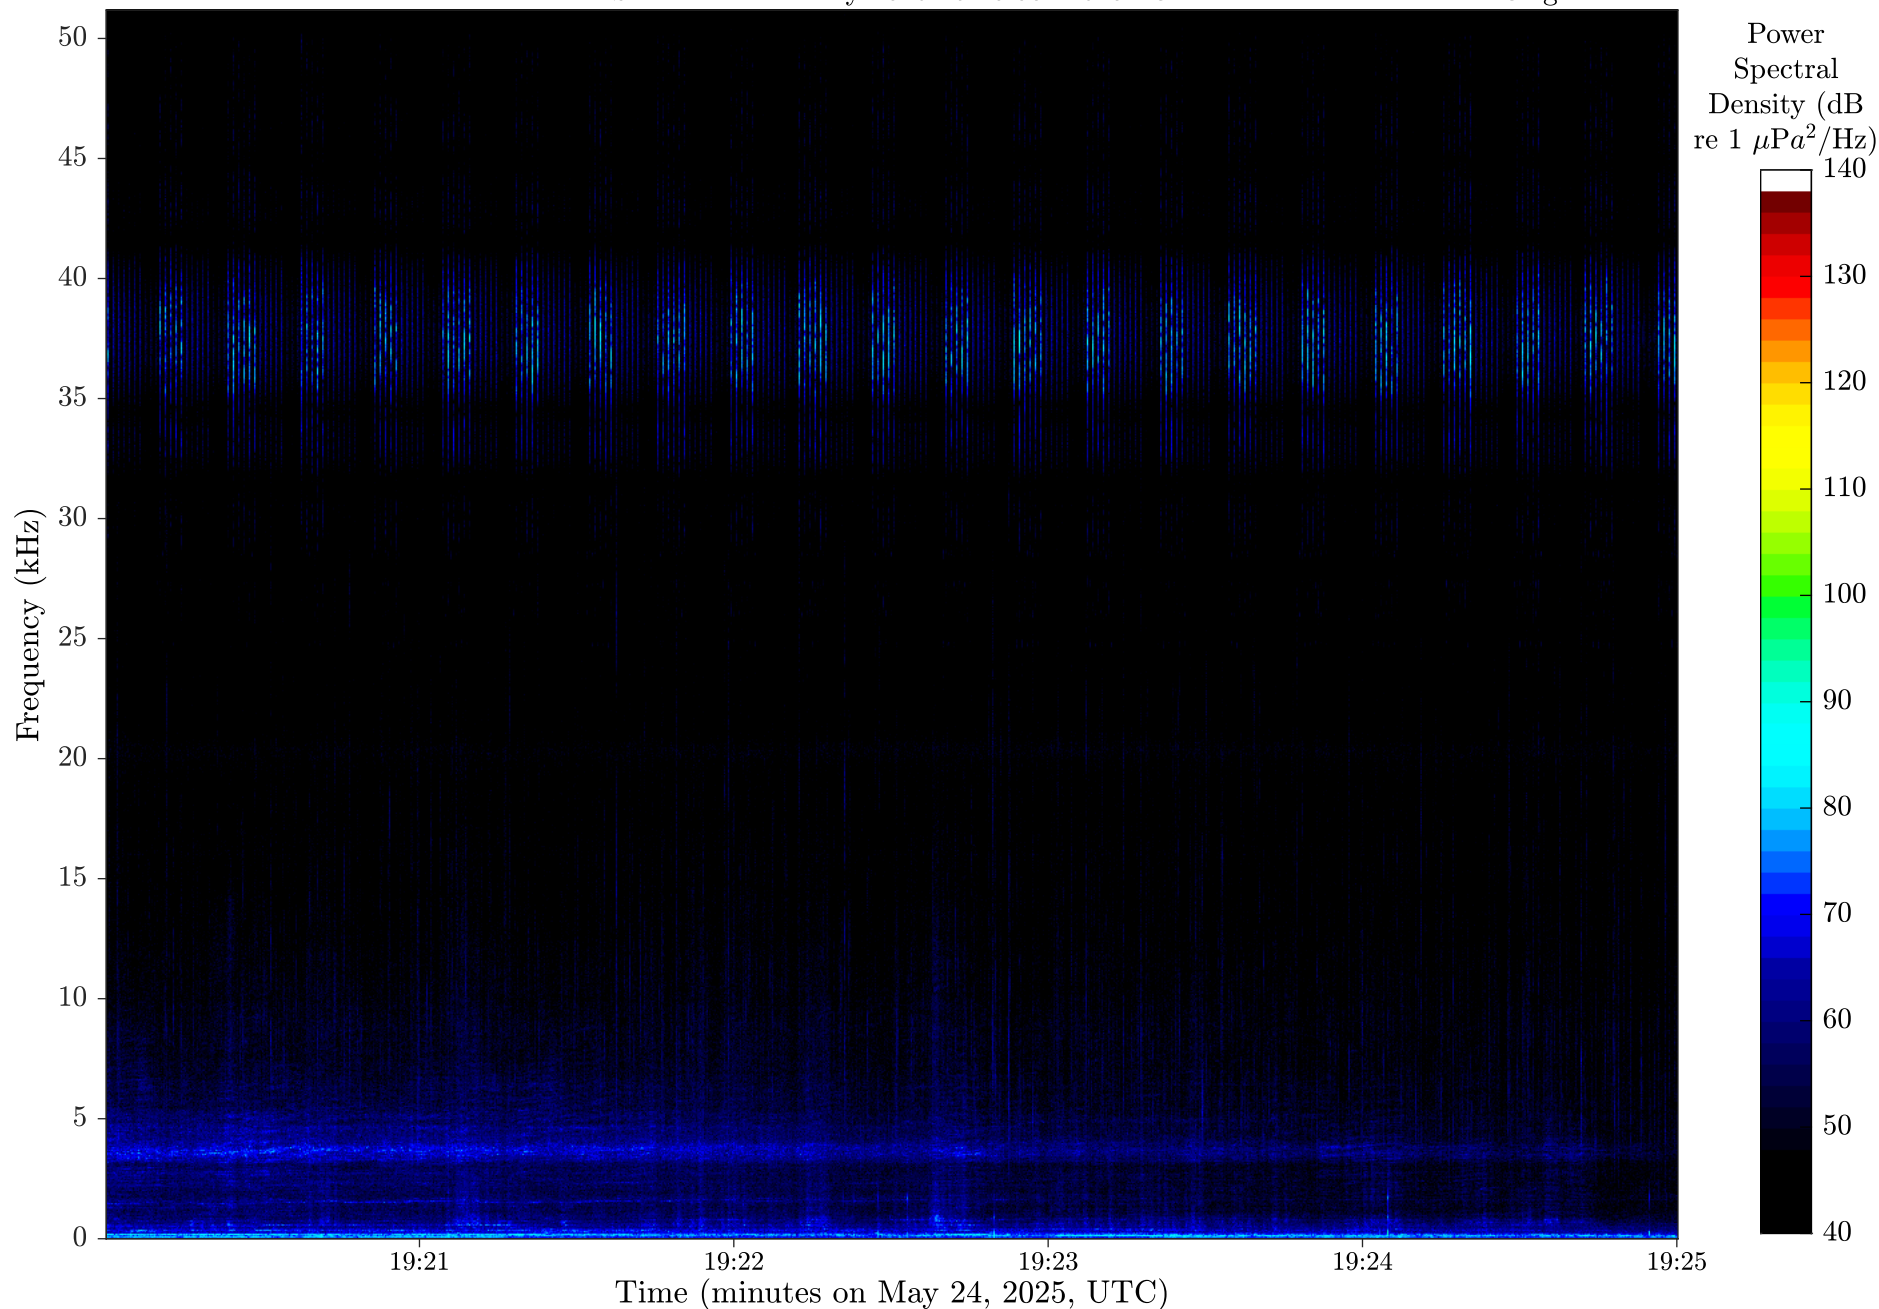

Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:50:33 UTC

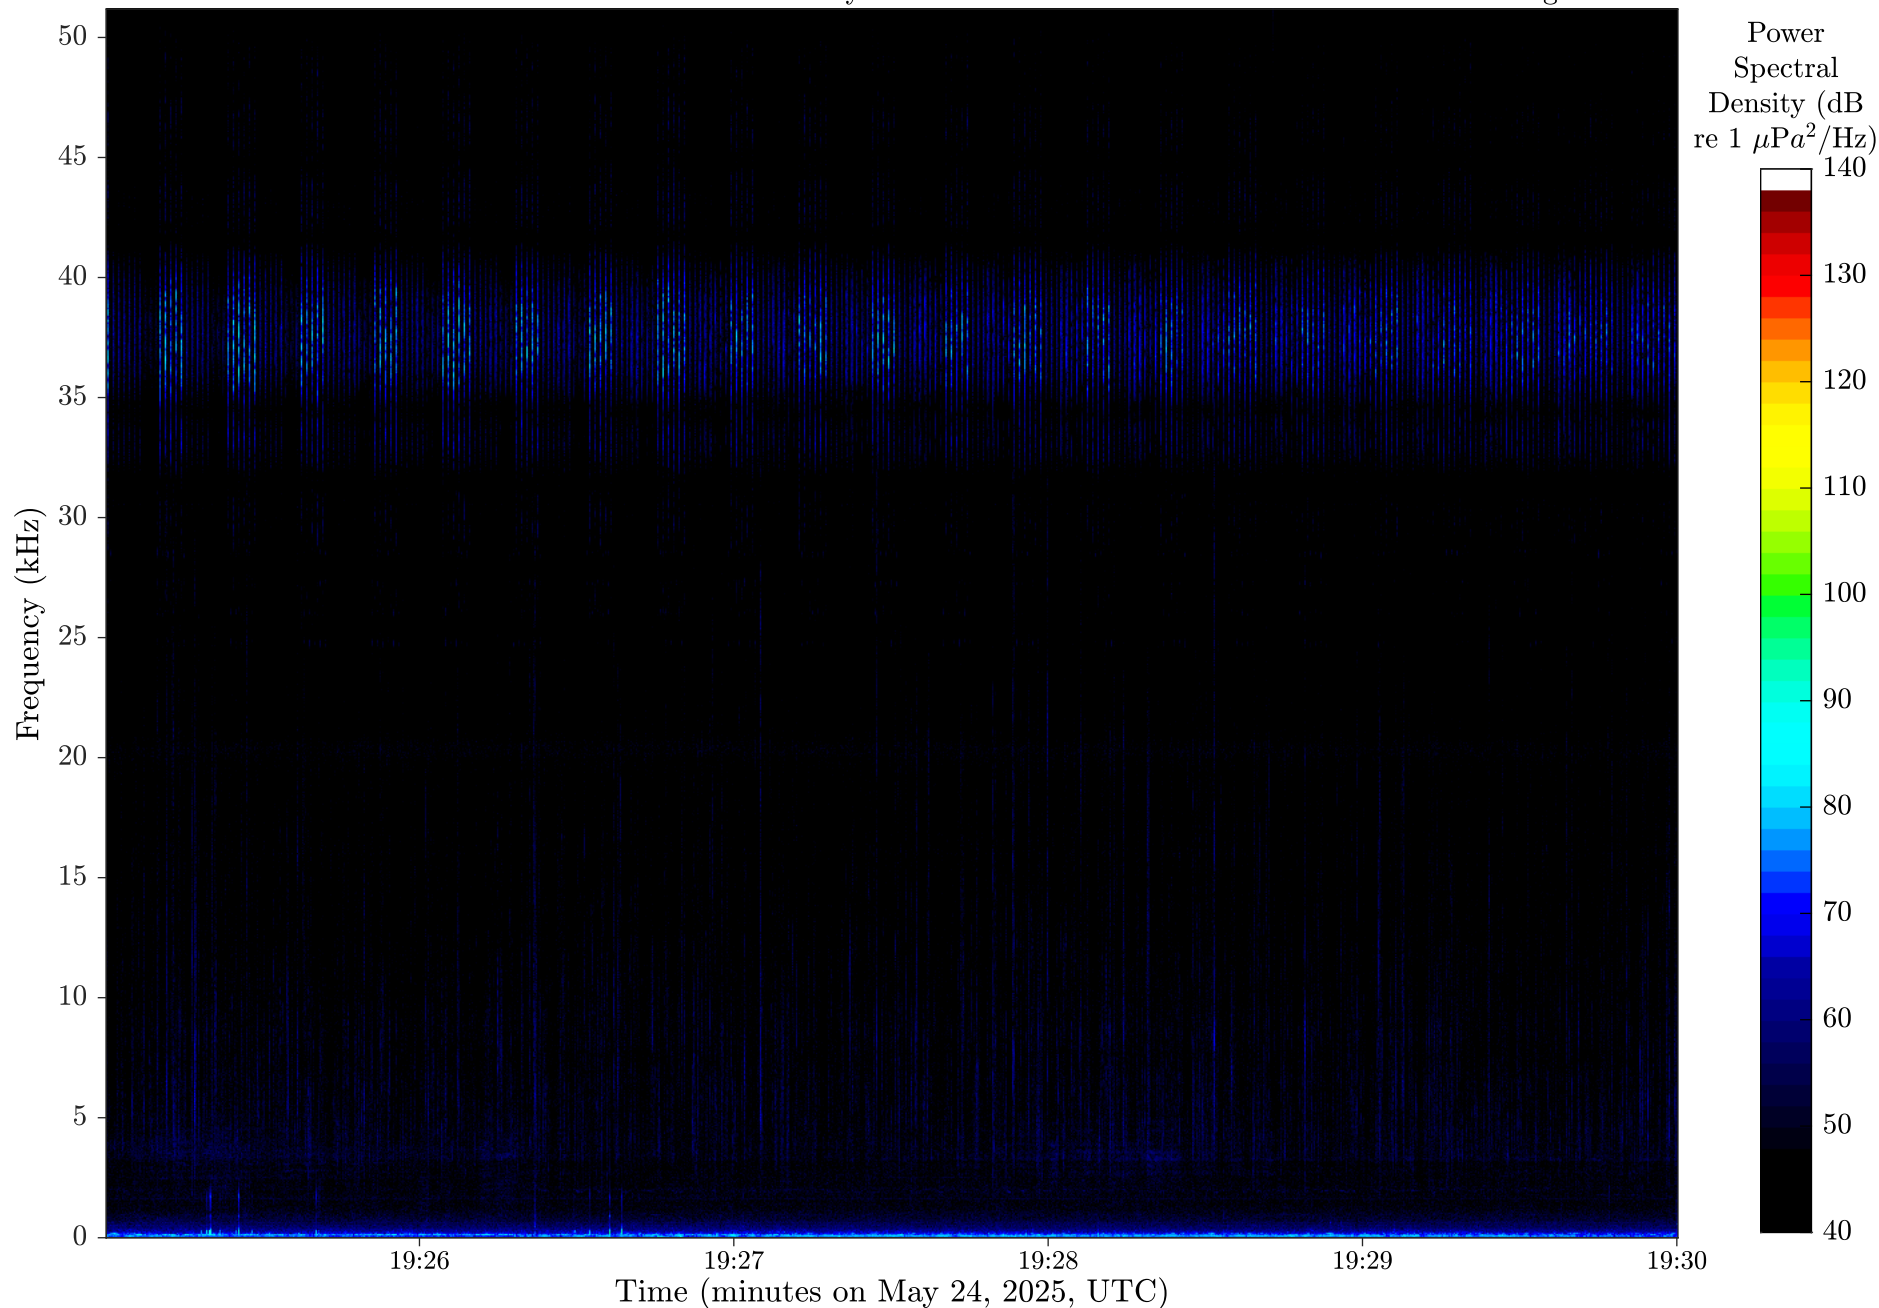


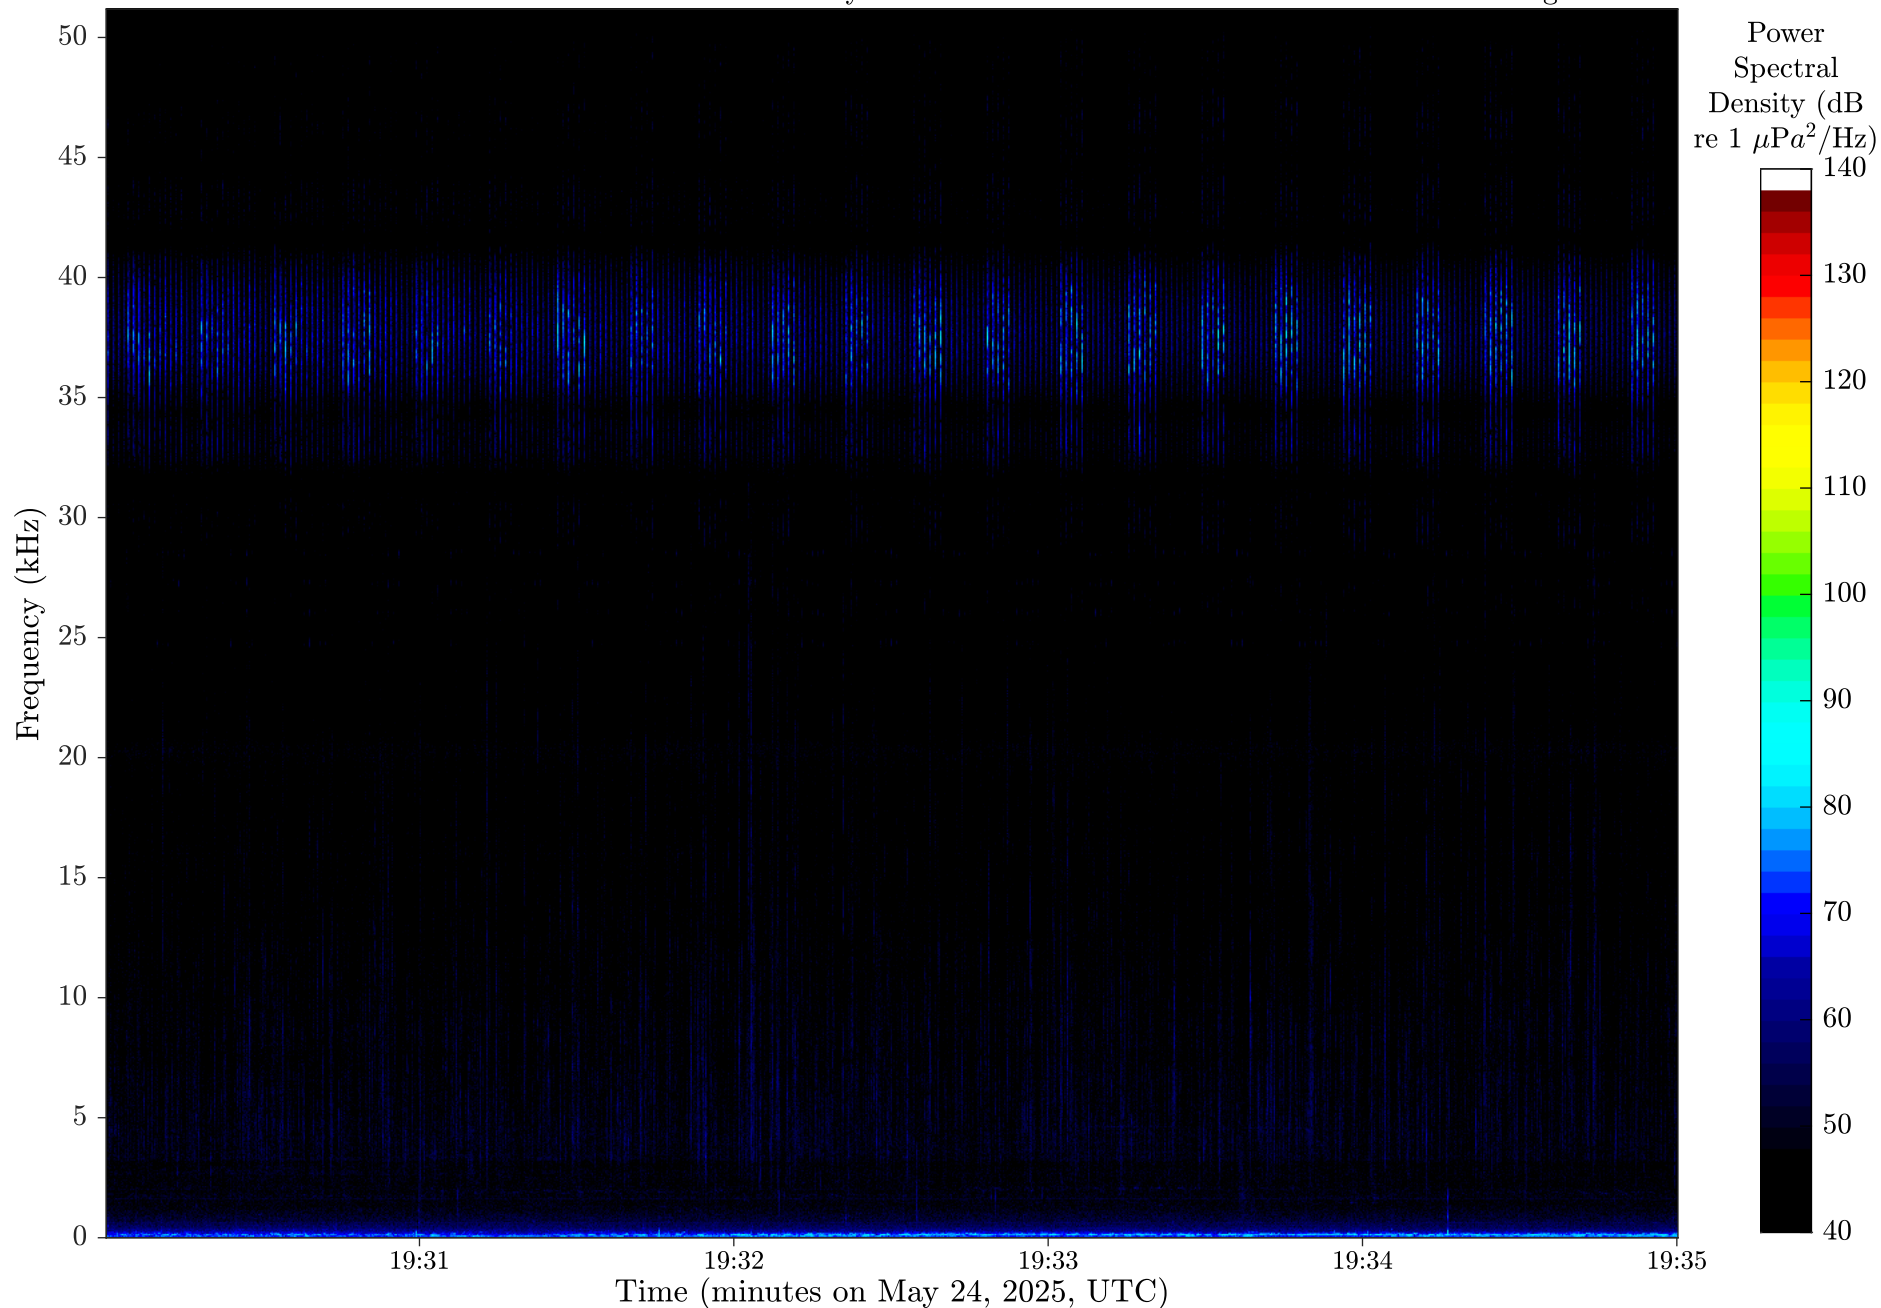

Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:50:50 UTC

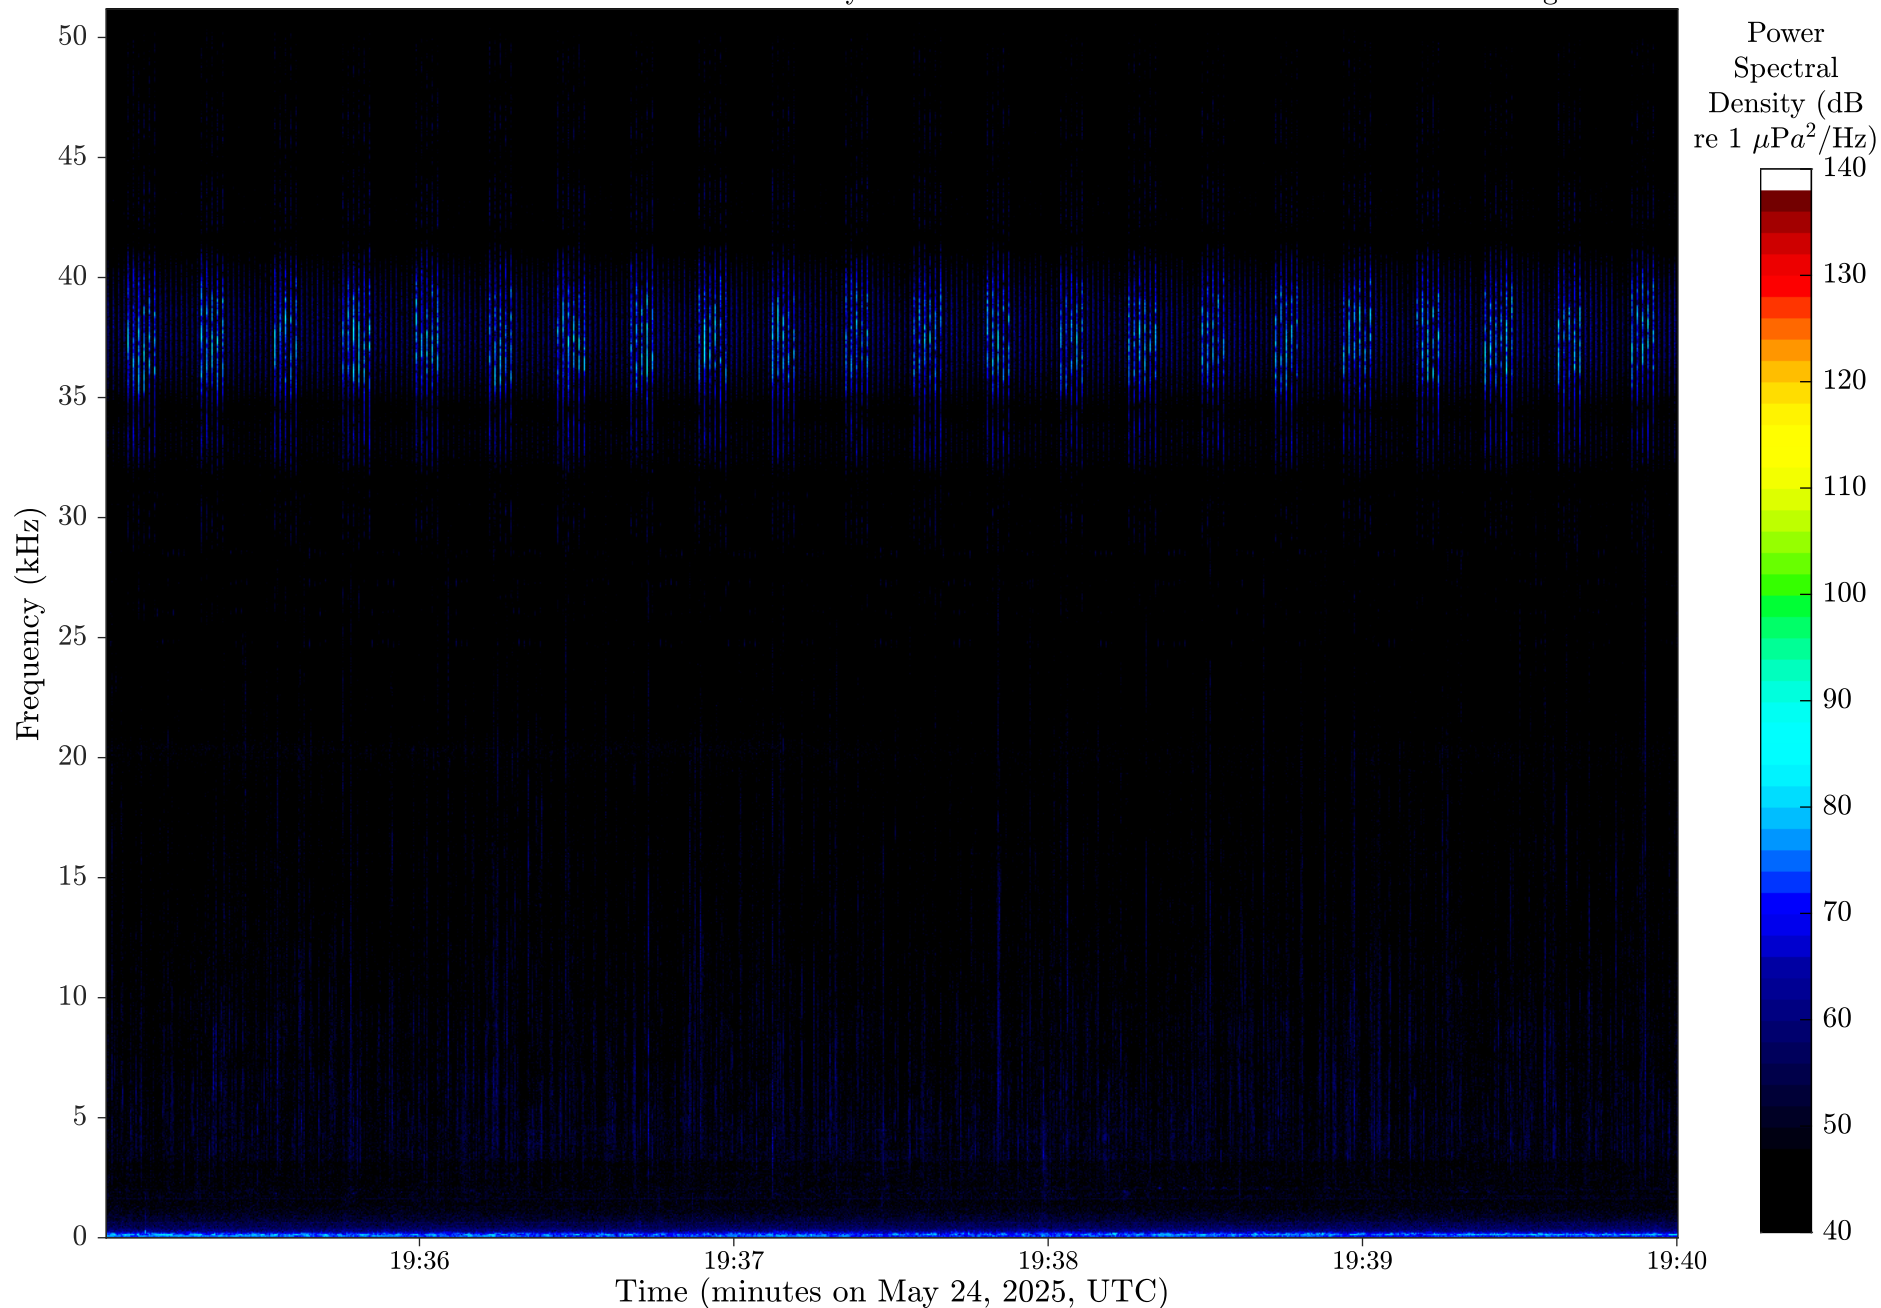


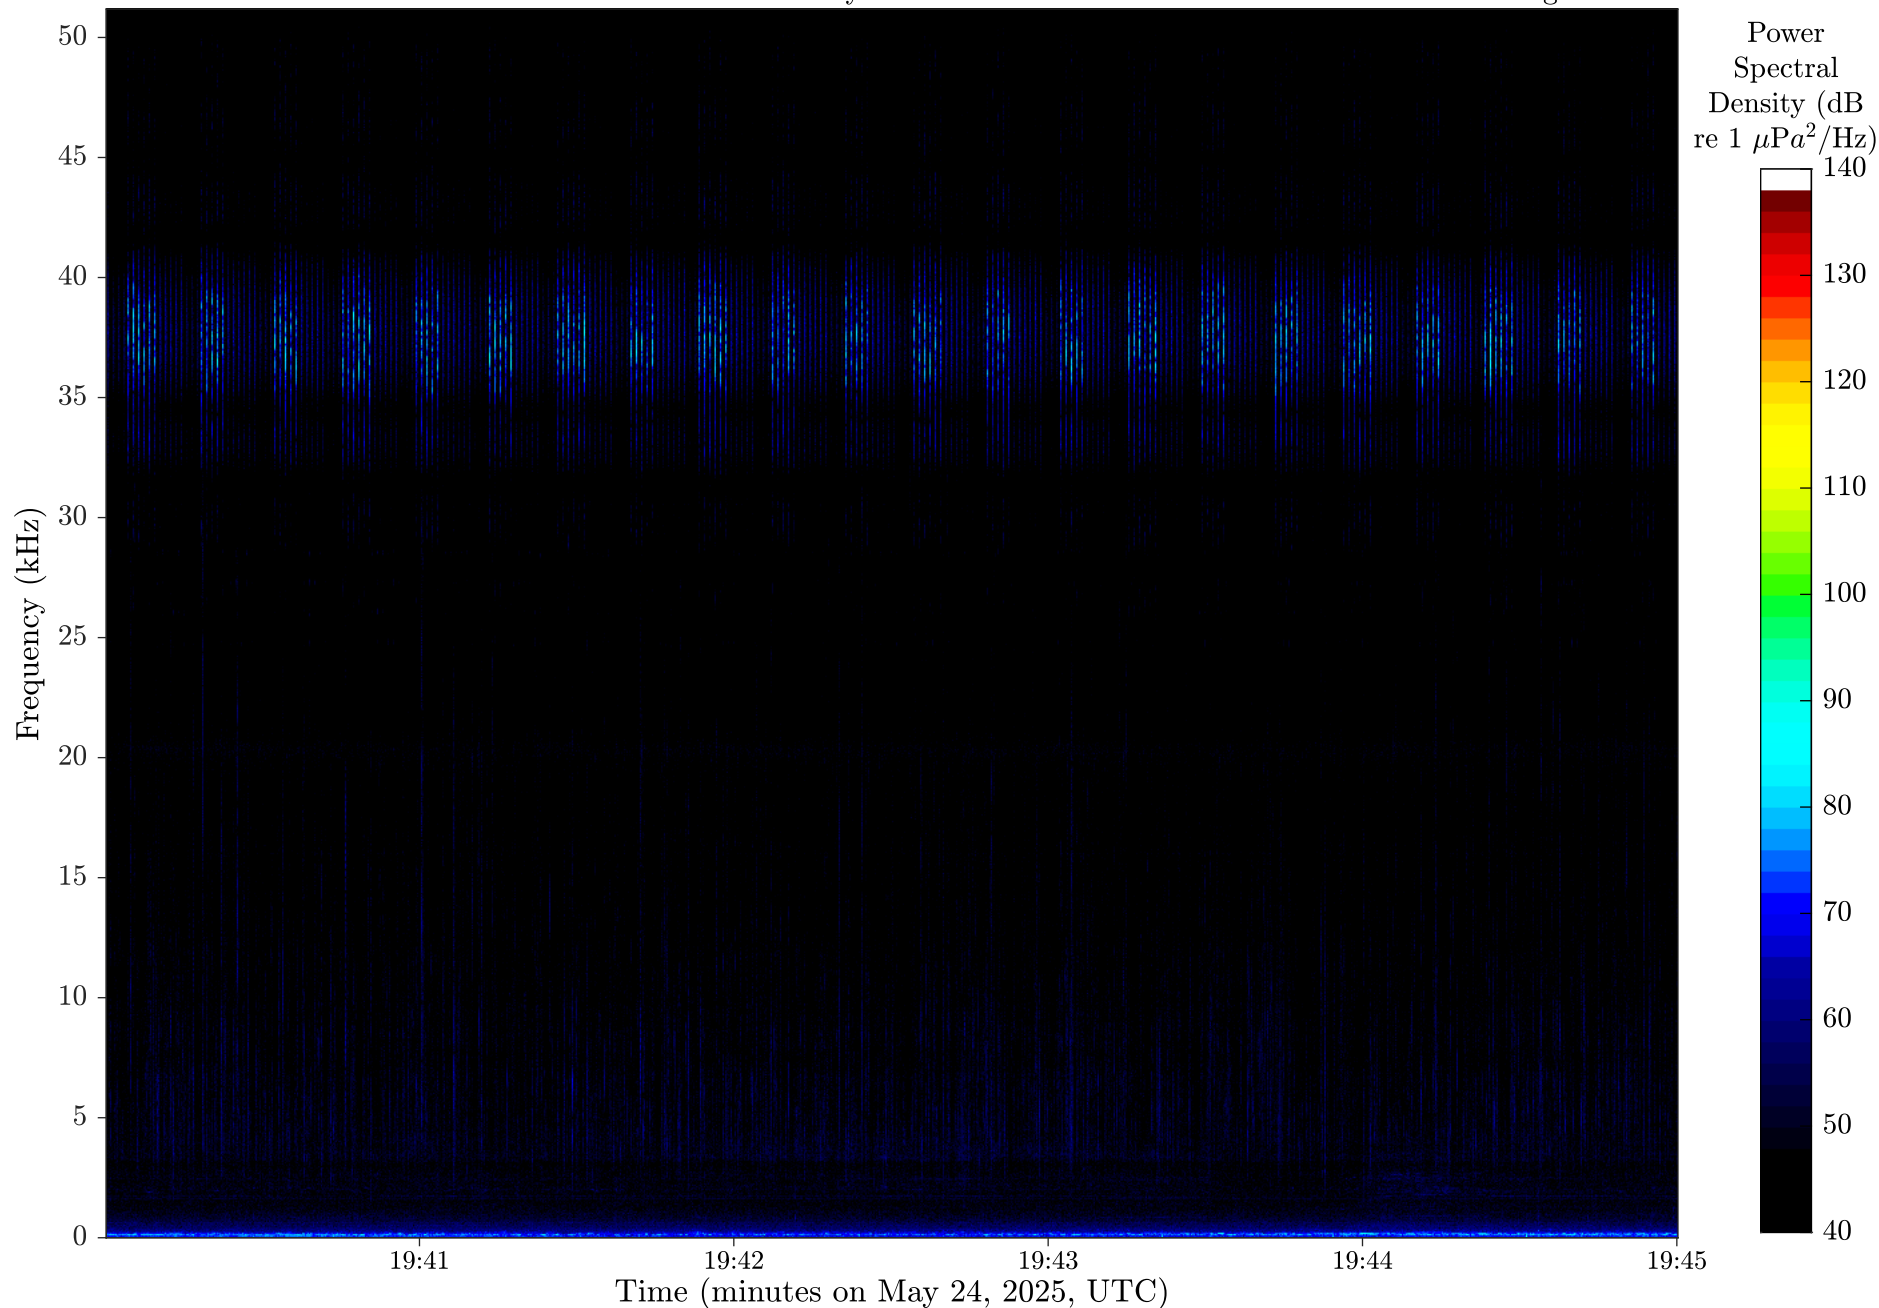

Comments: 34.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:51:06 UTC

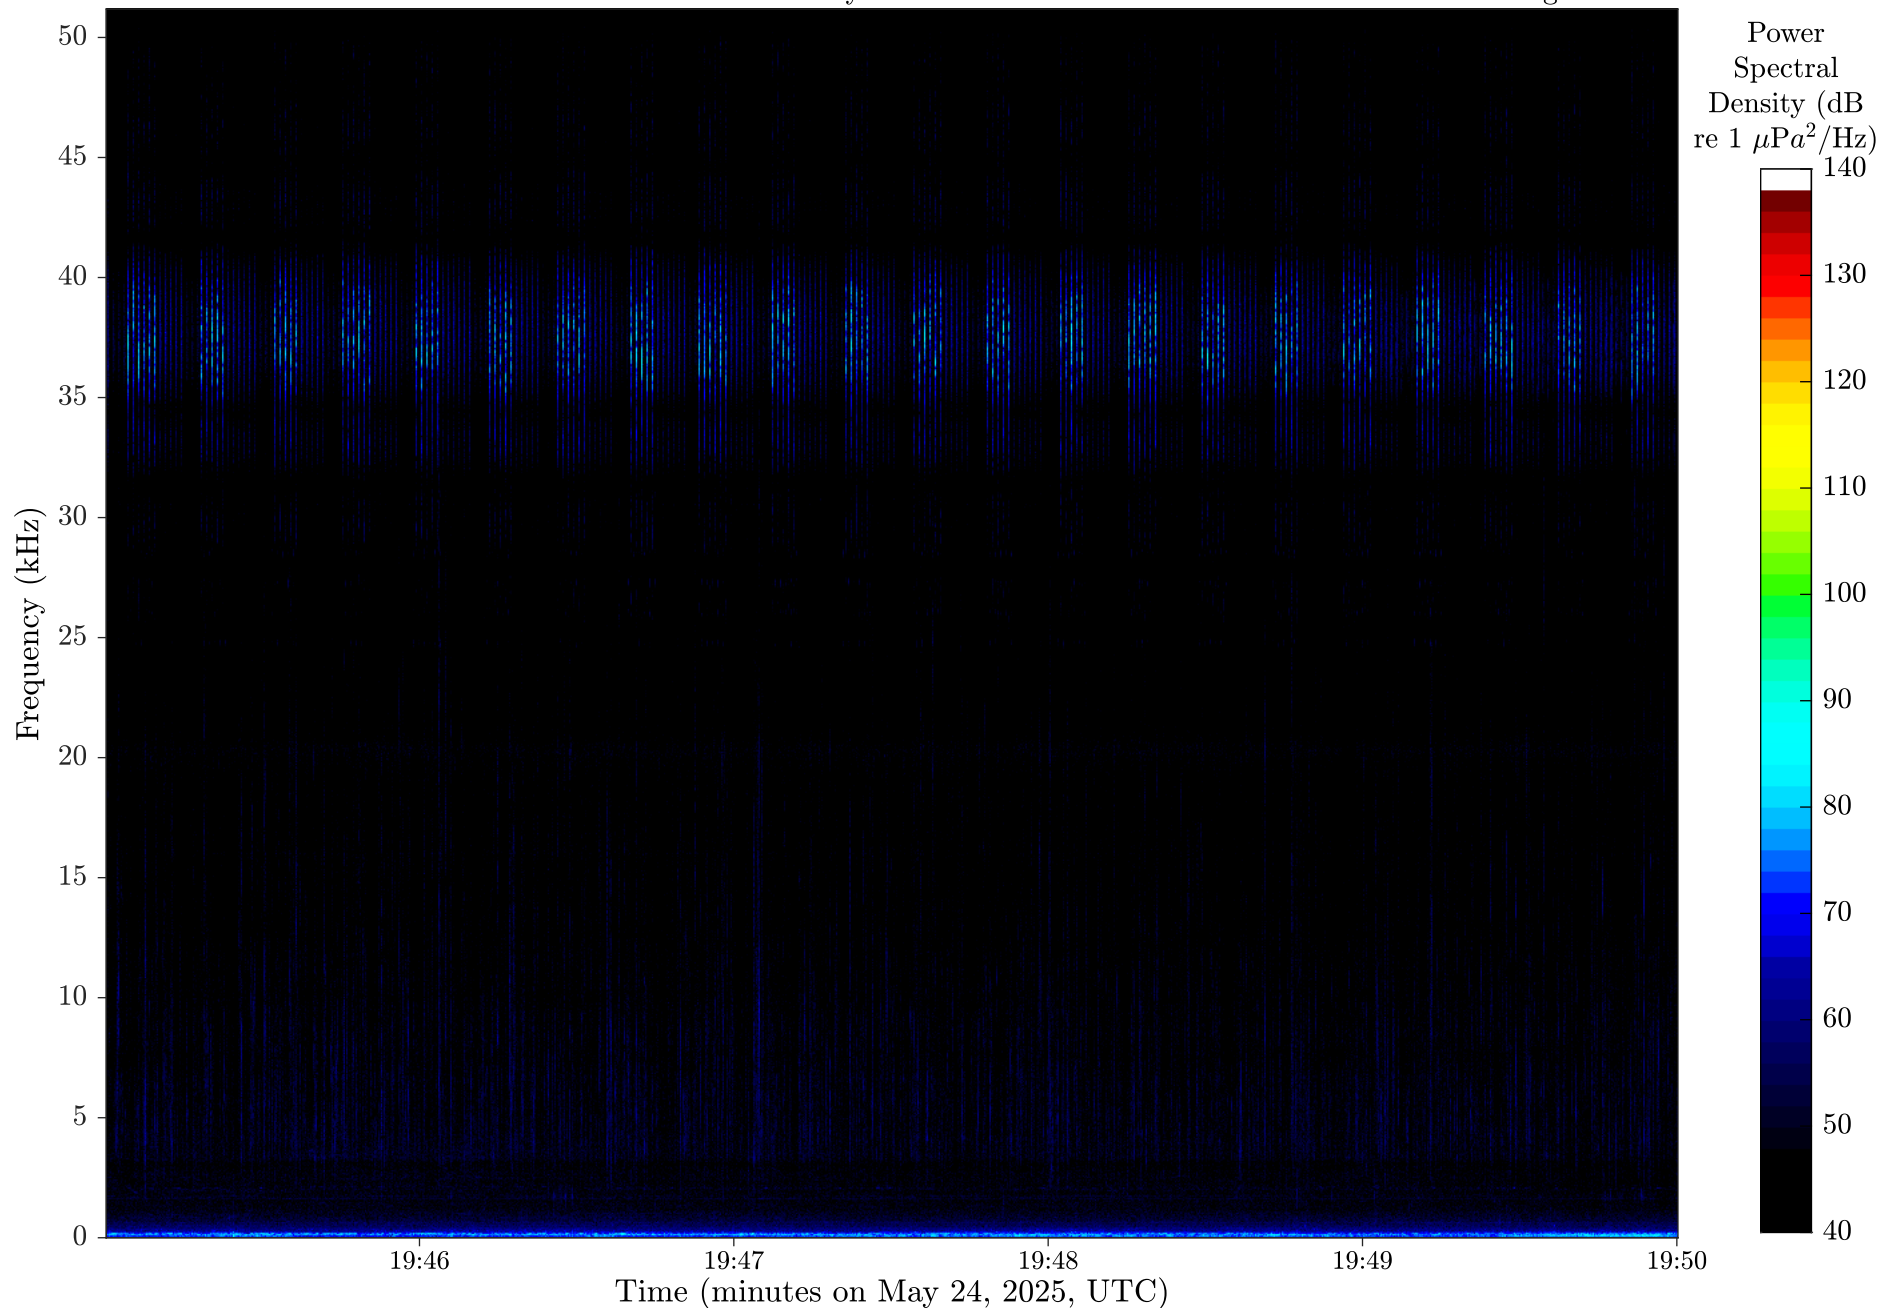

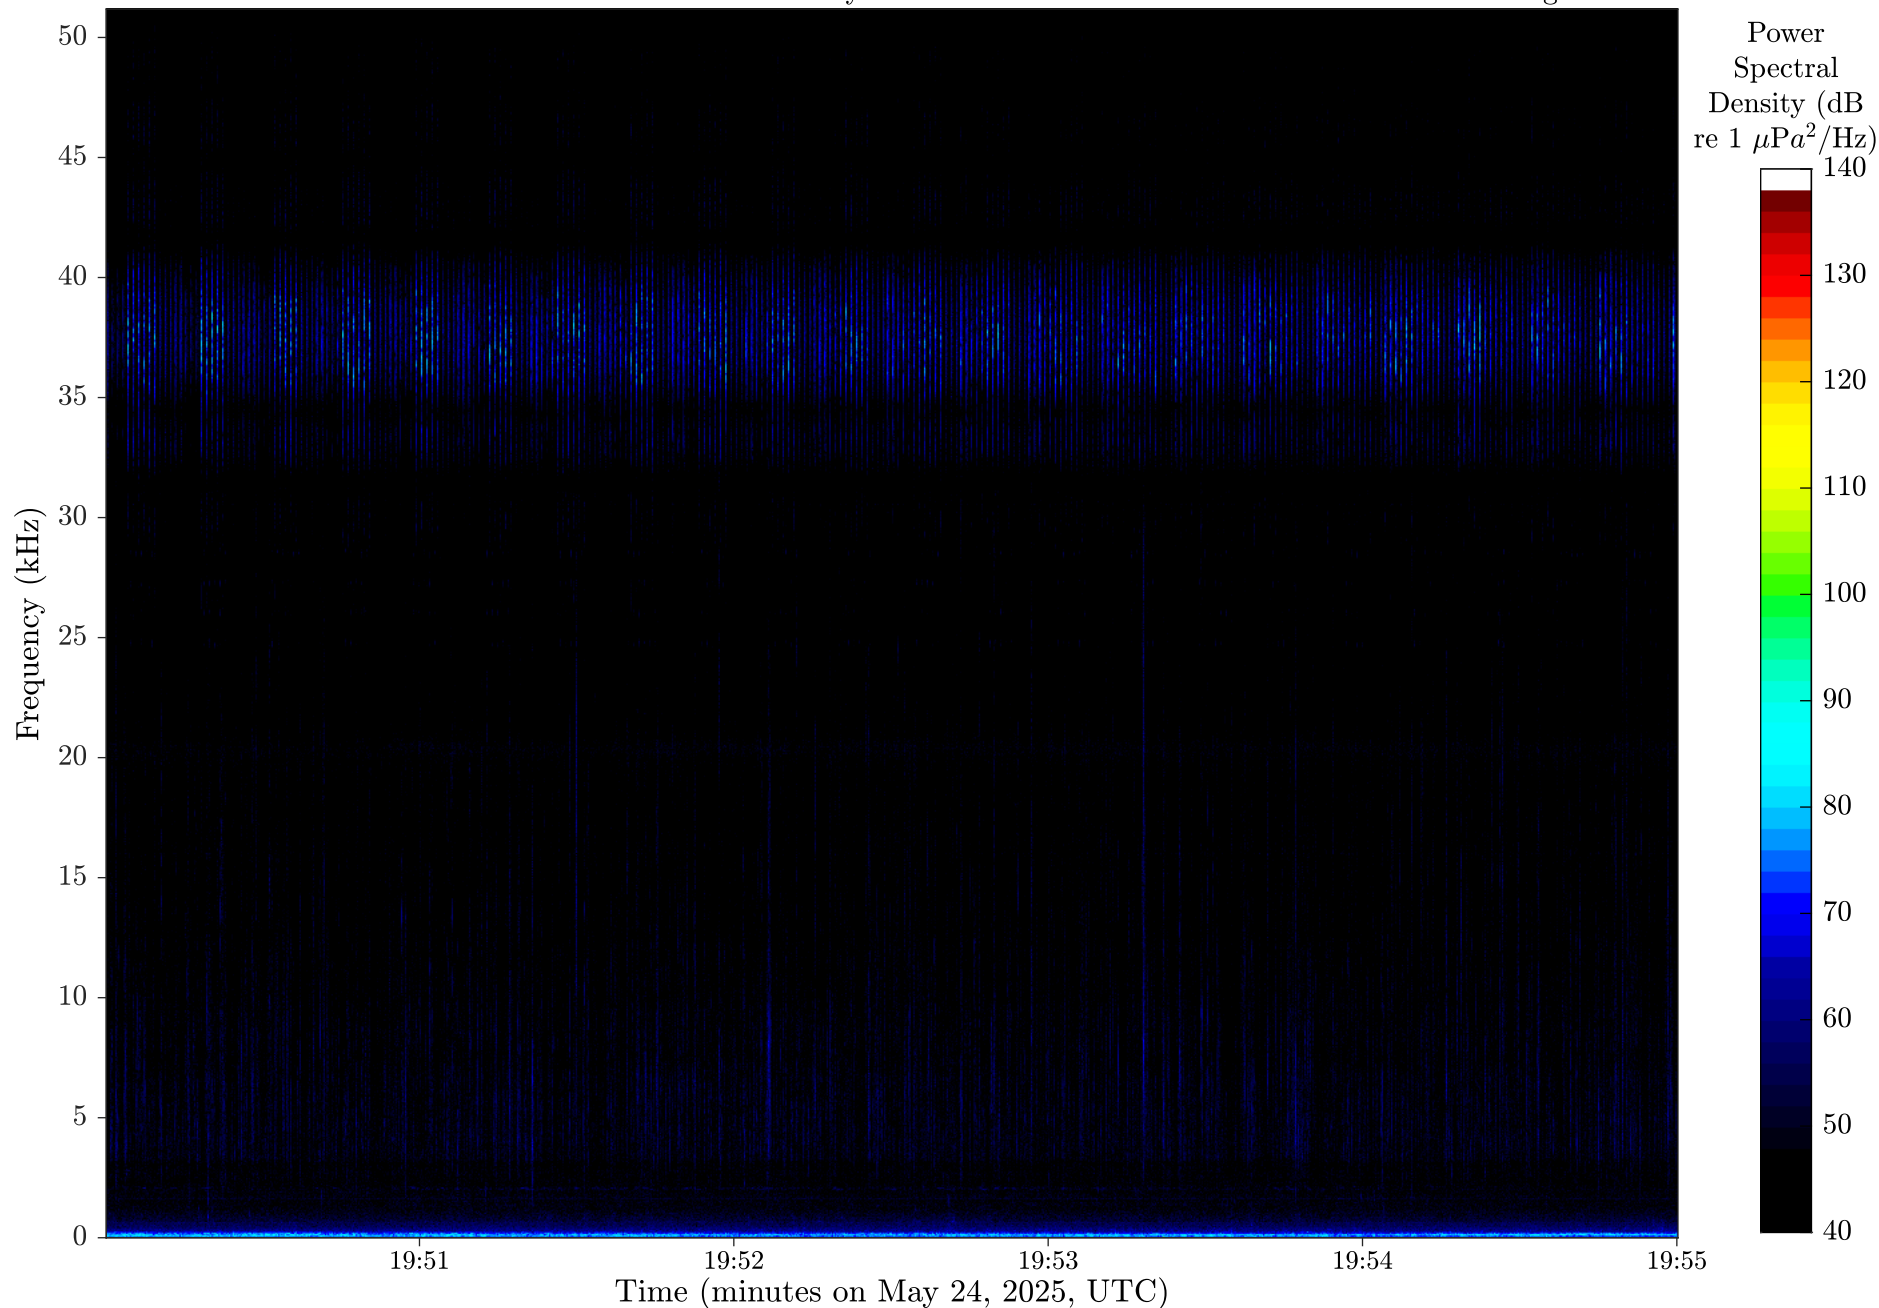


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:51:22 UTC

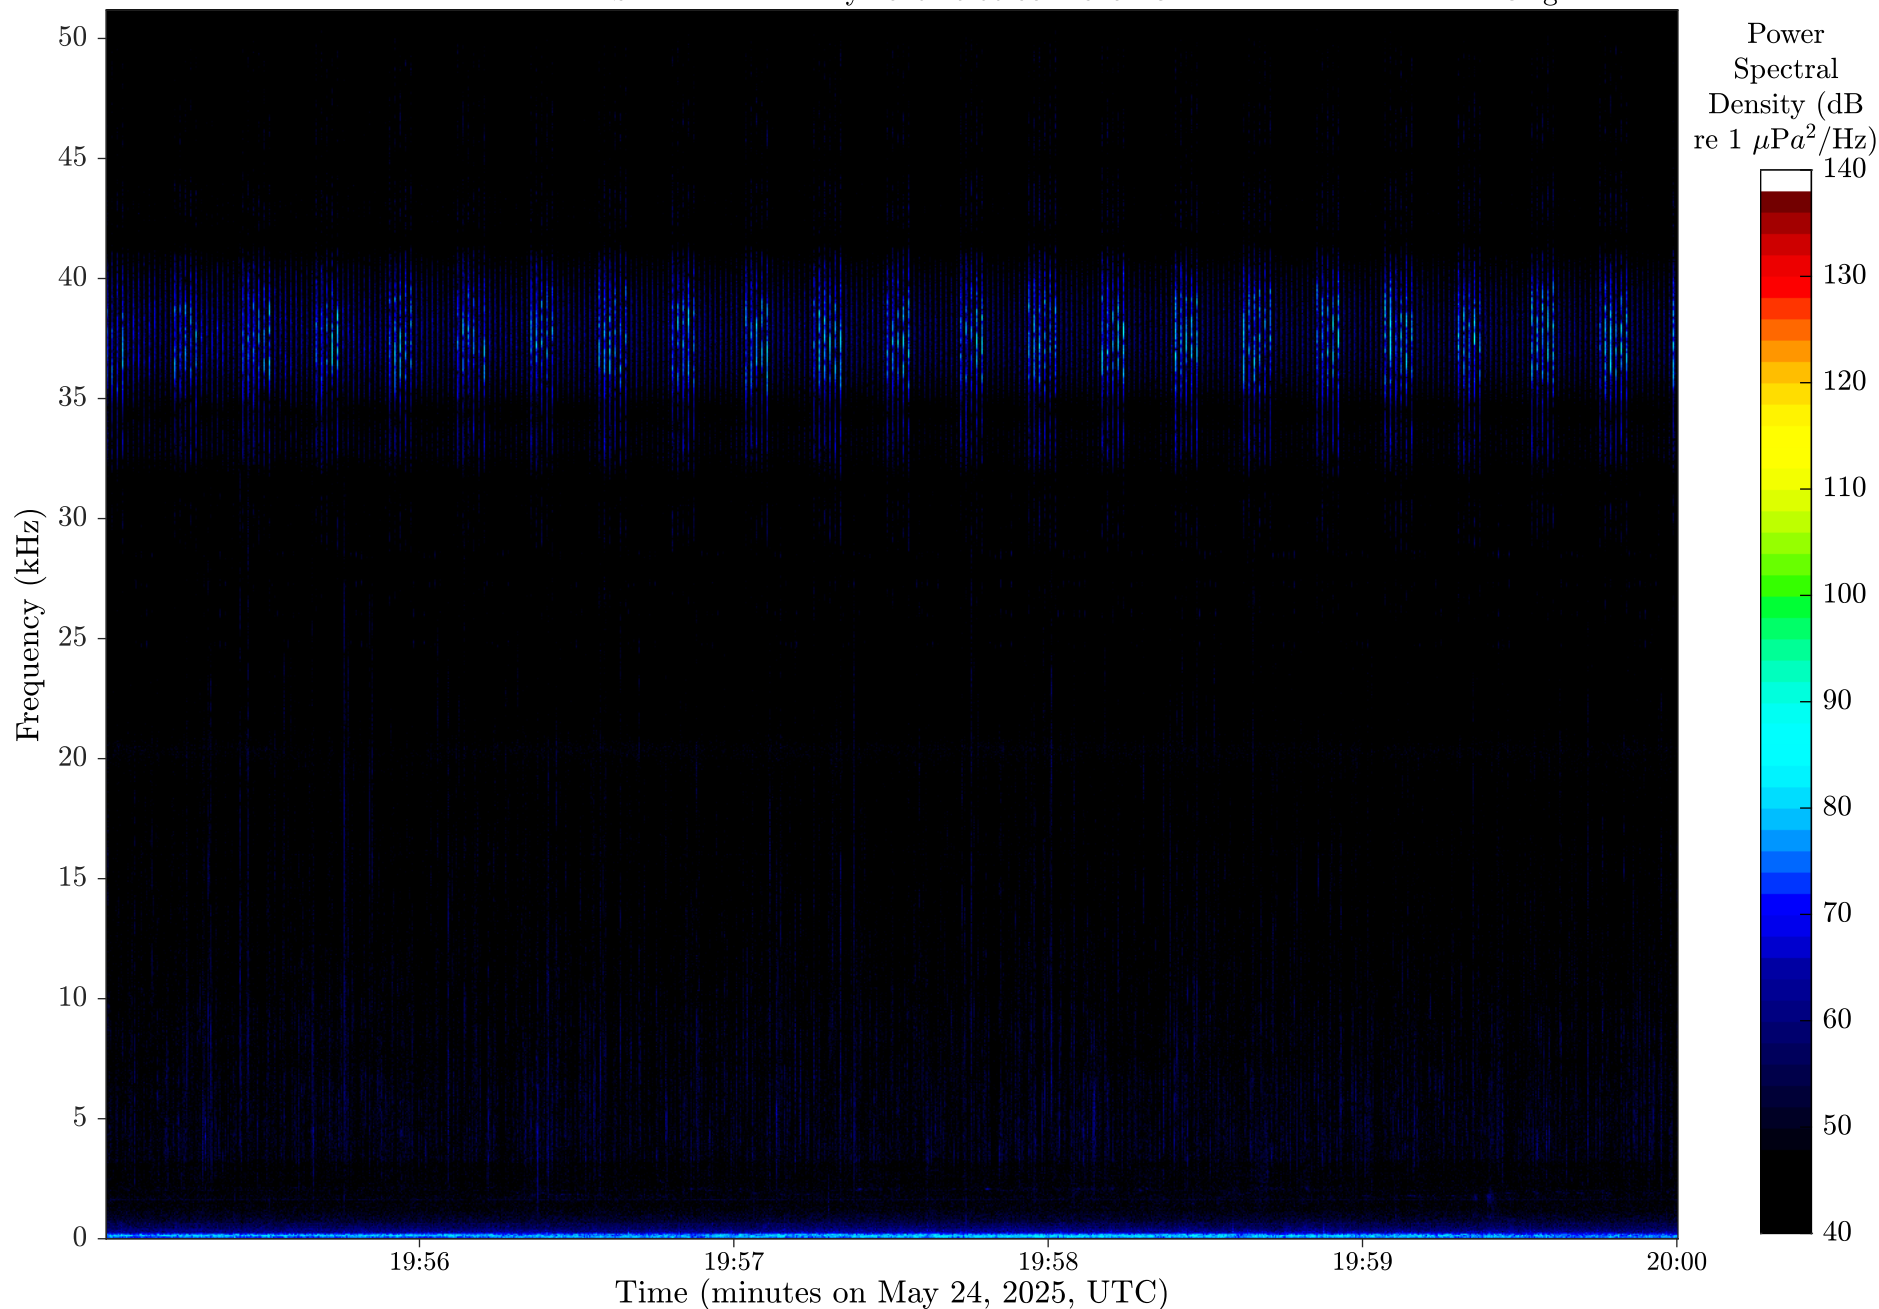


Comments: 34.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:51:30 UTC

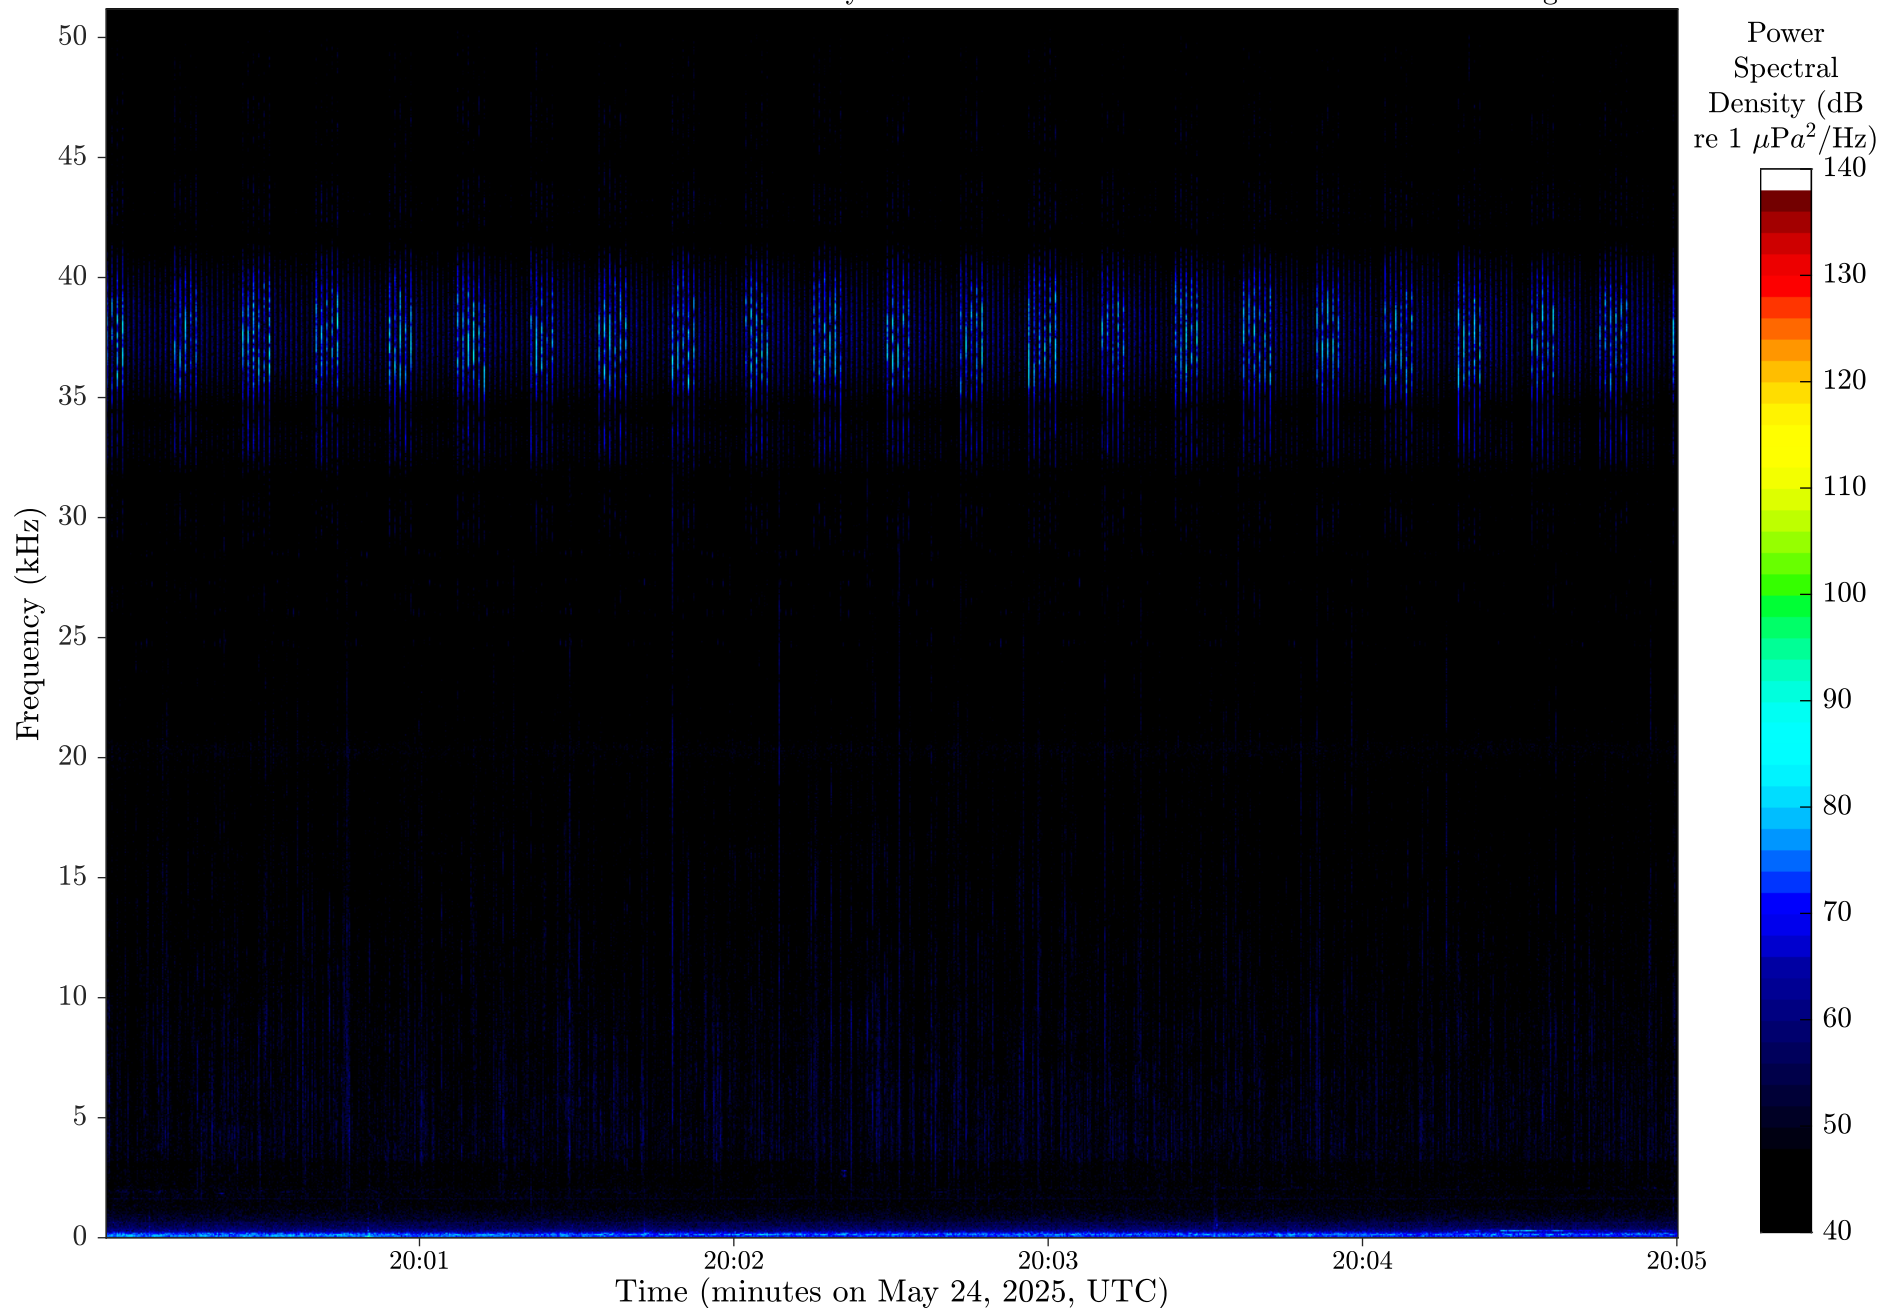



Comments: 35 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:51:38 UTC

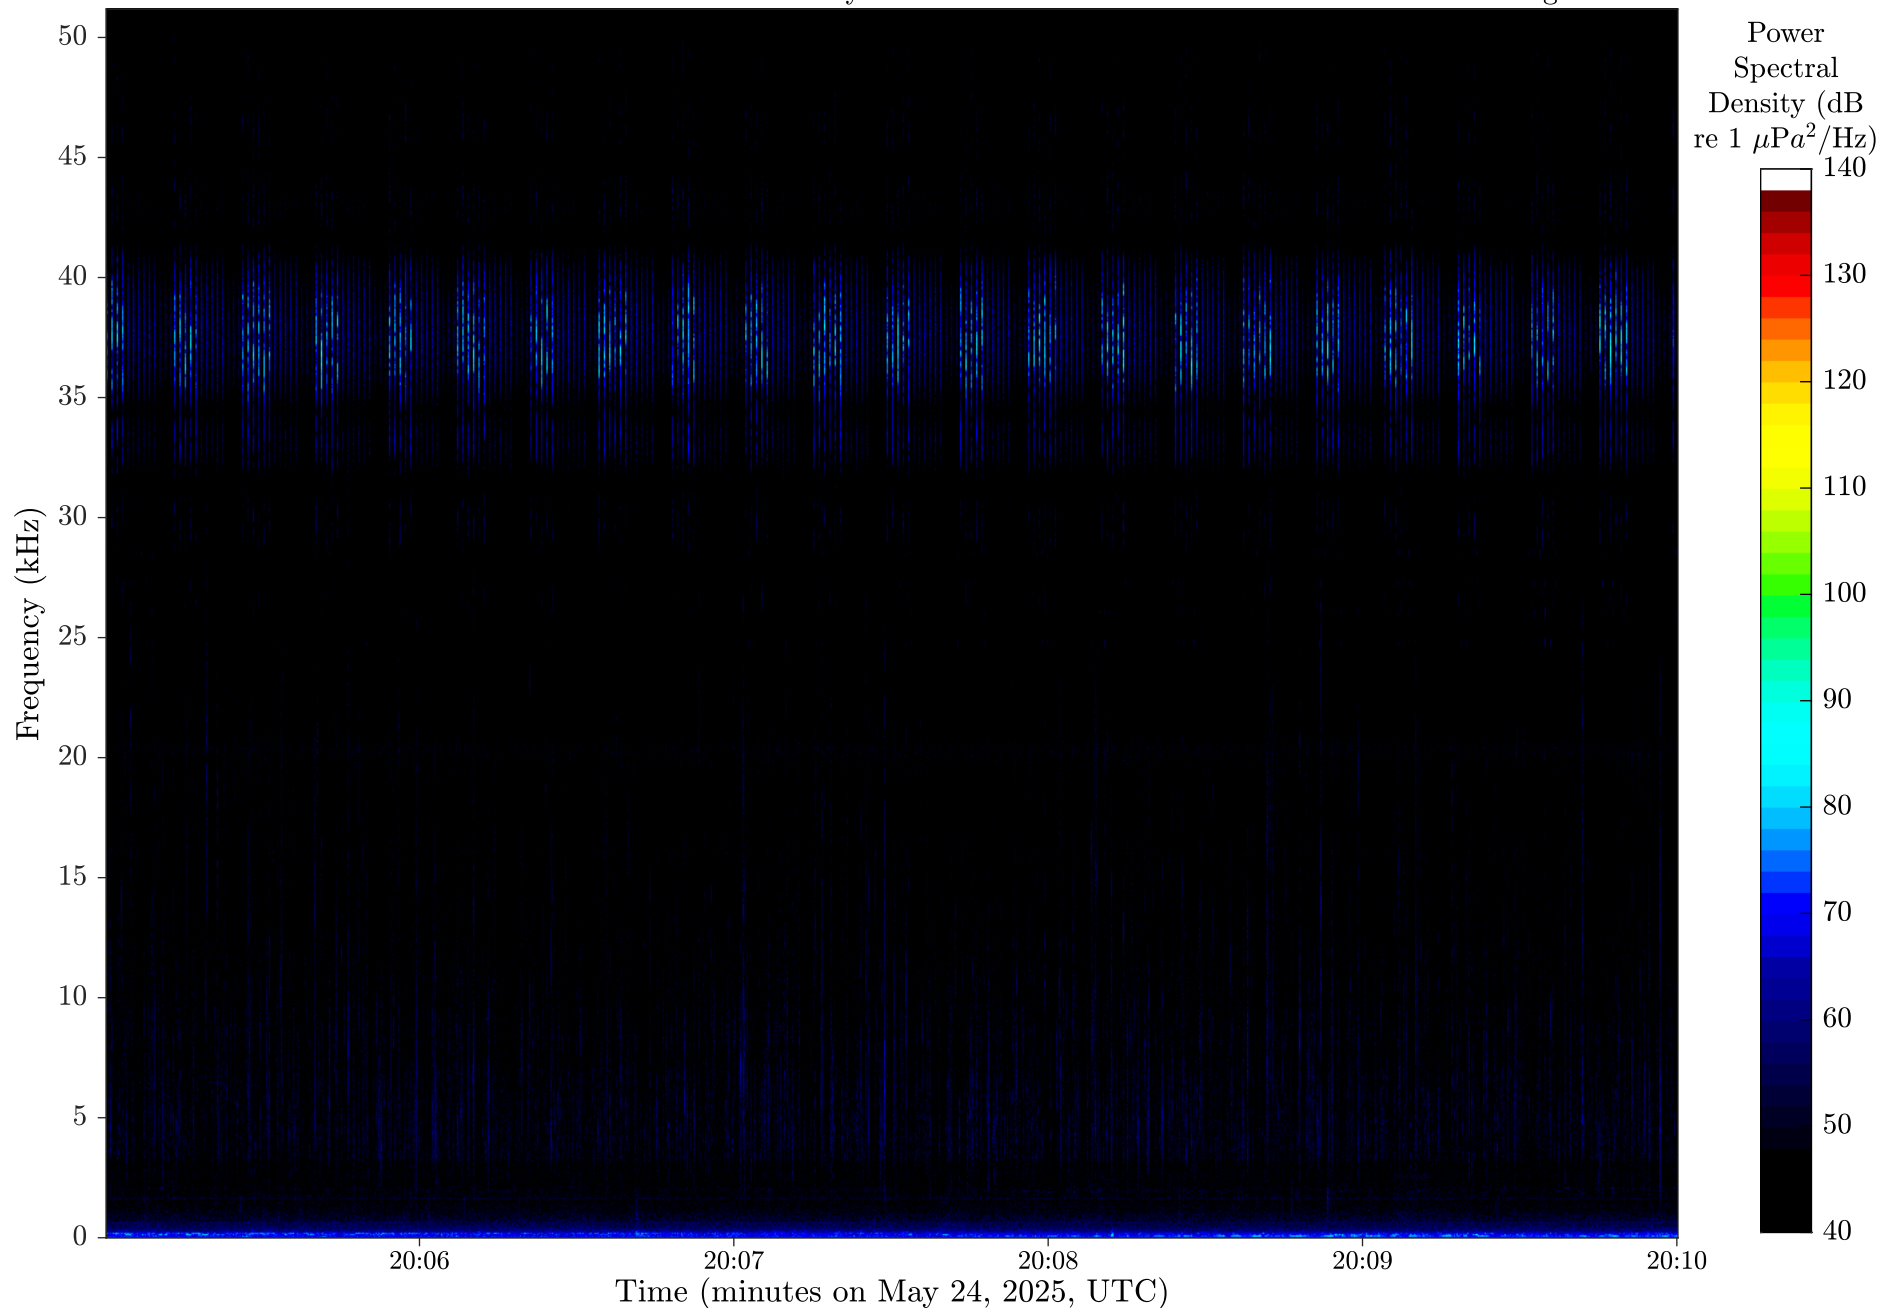

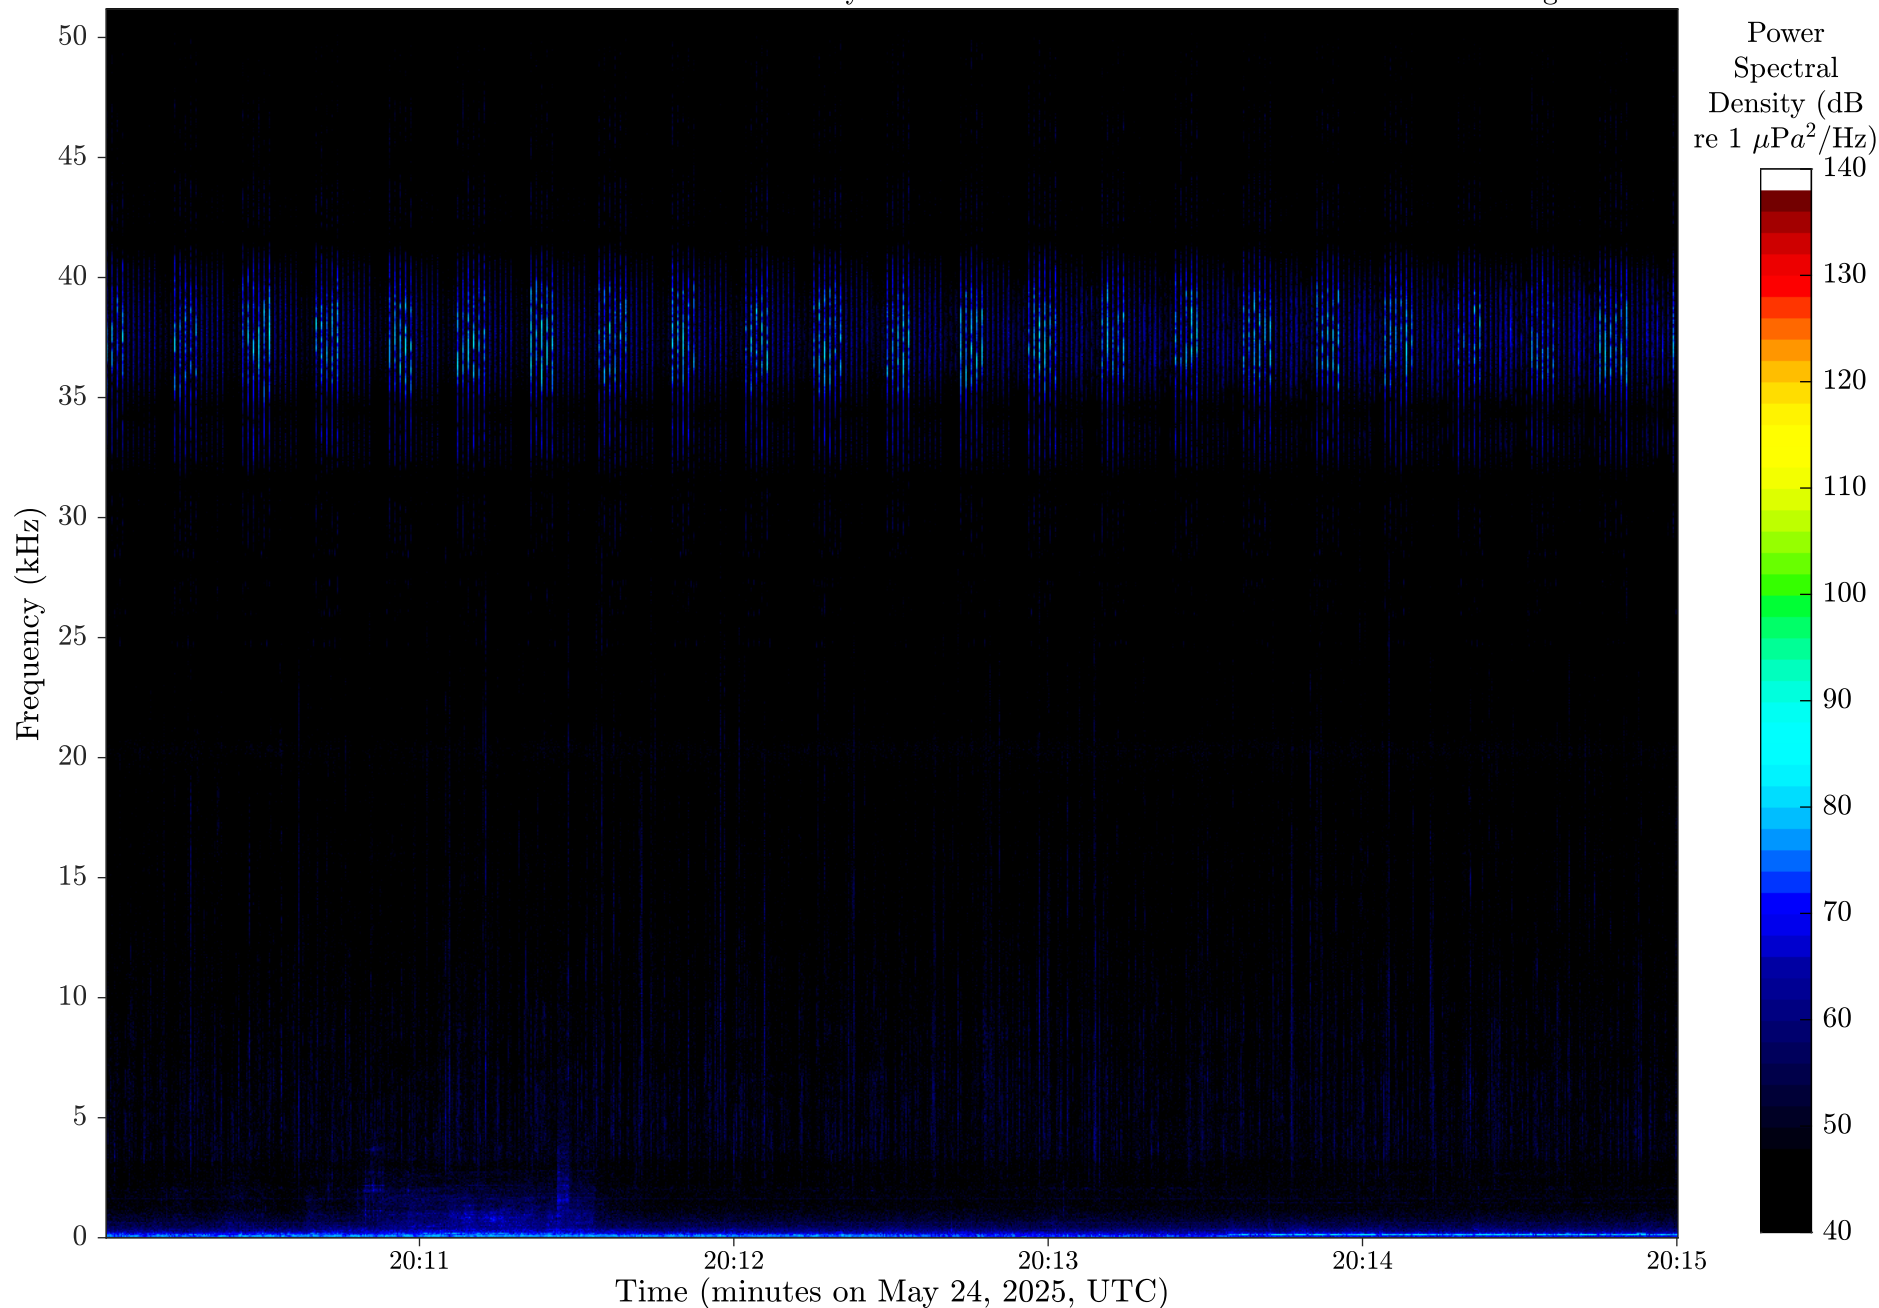


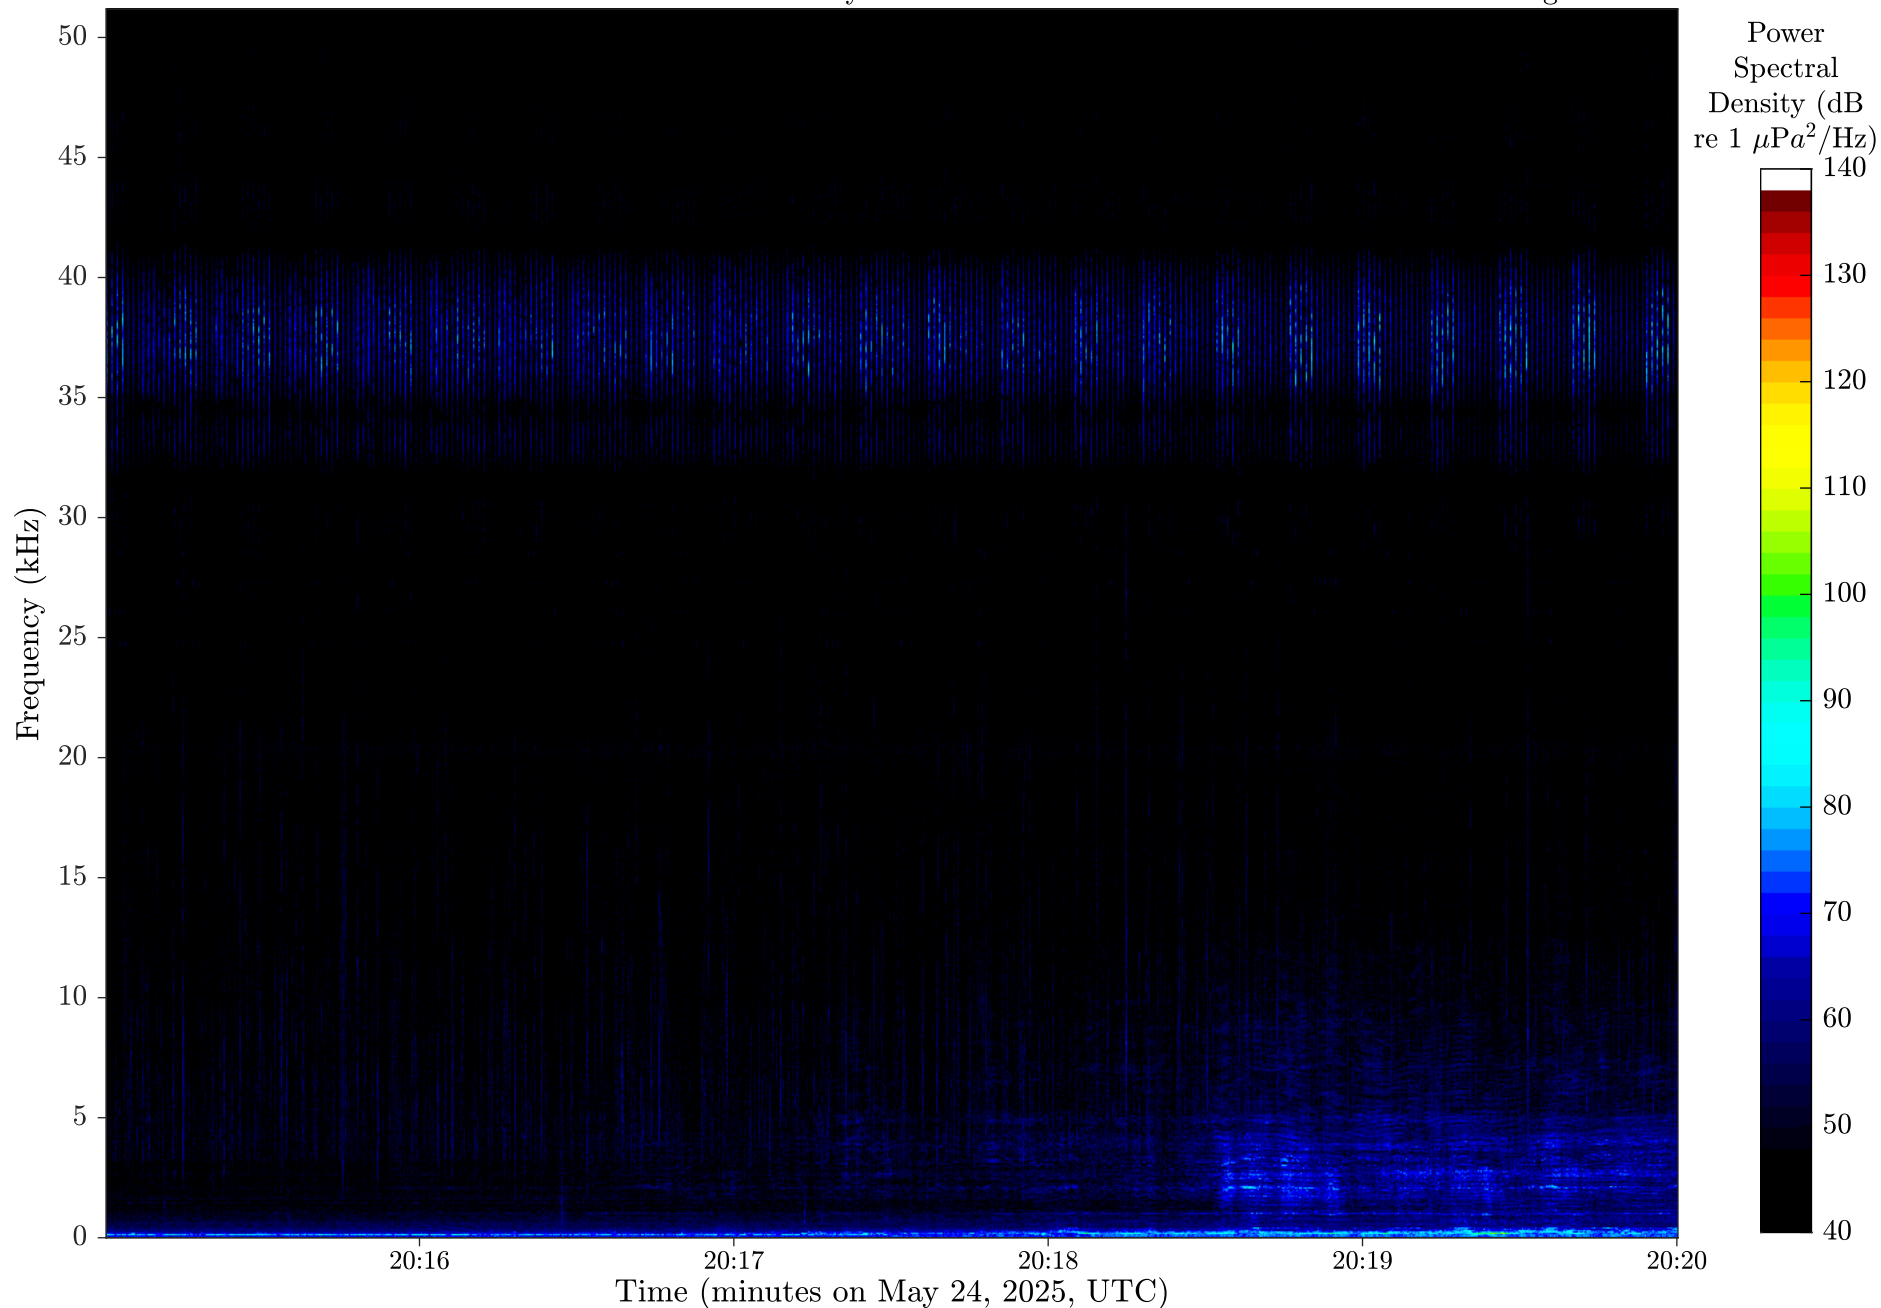

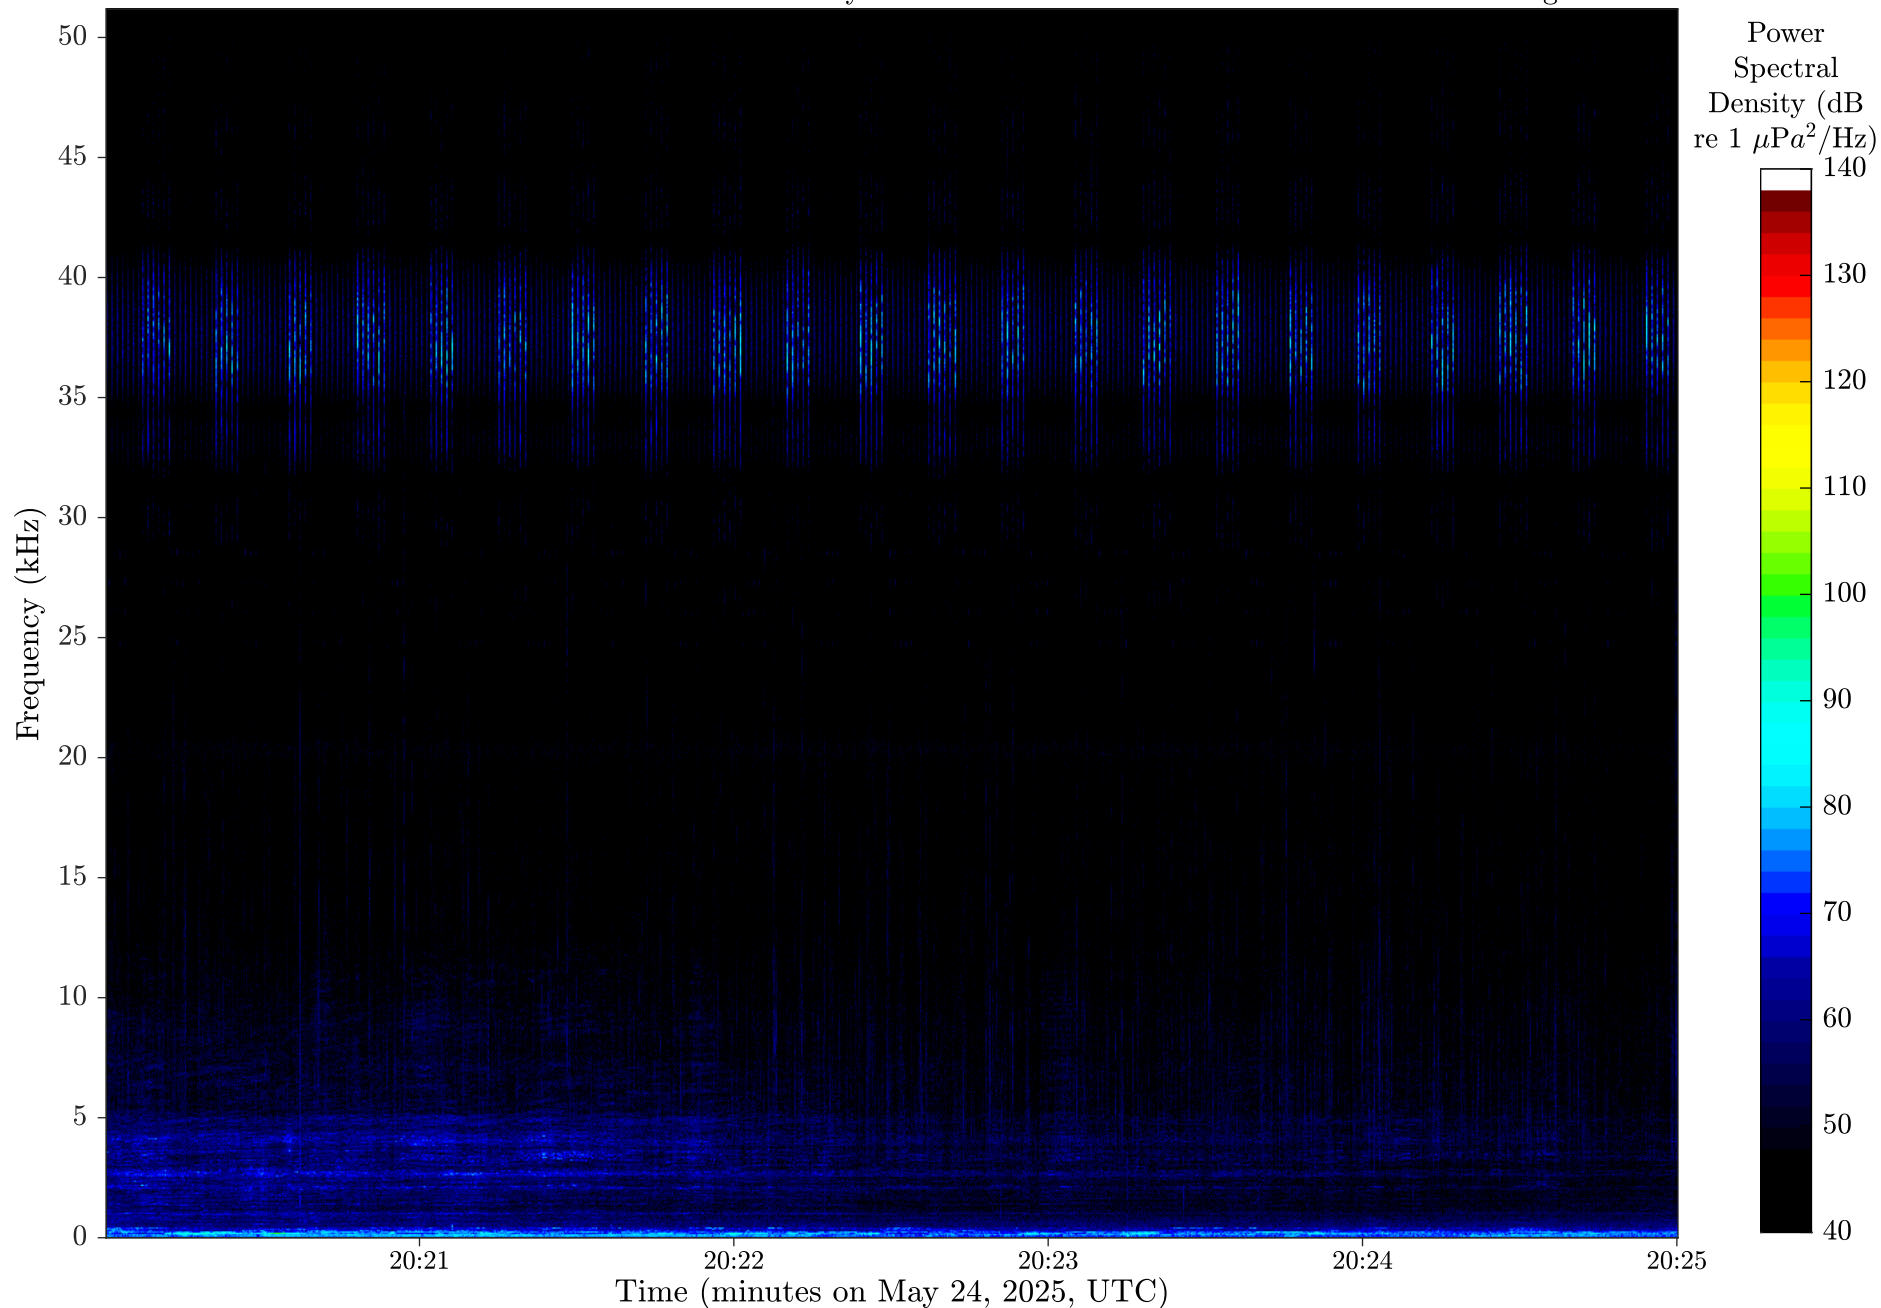


Comments: 33.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:52:13 UTC

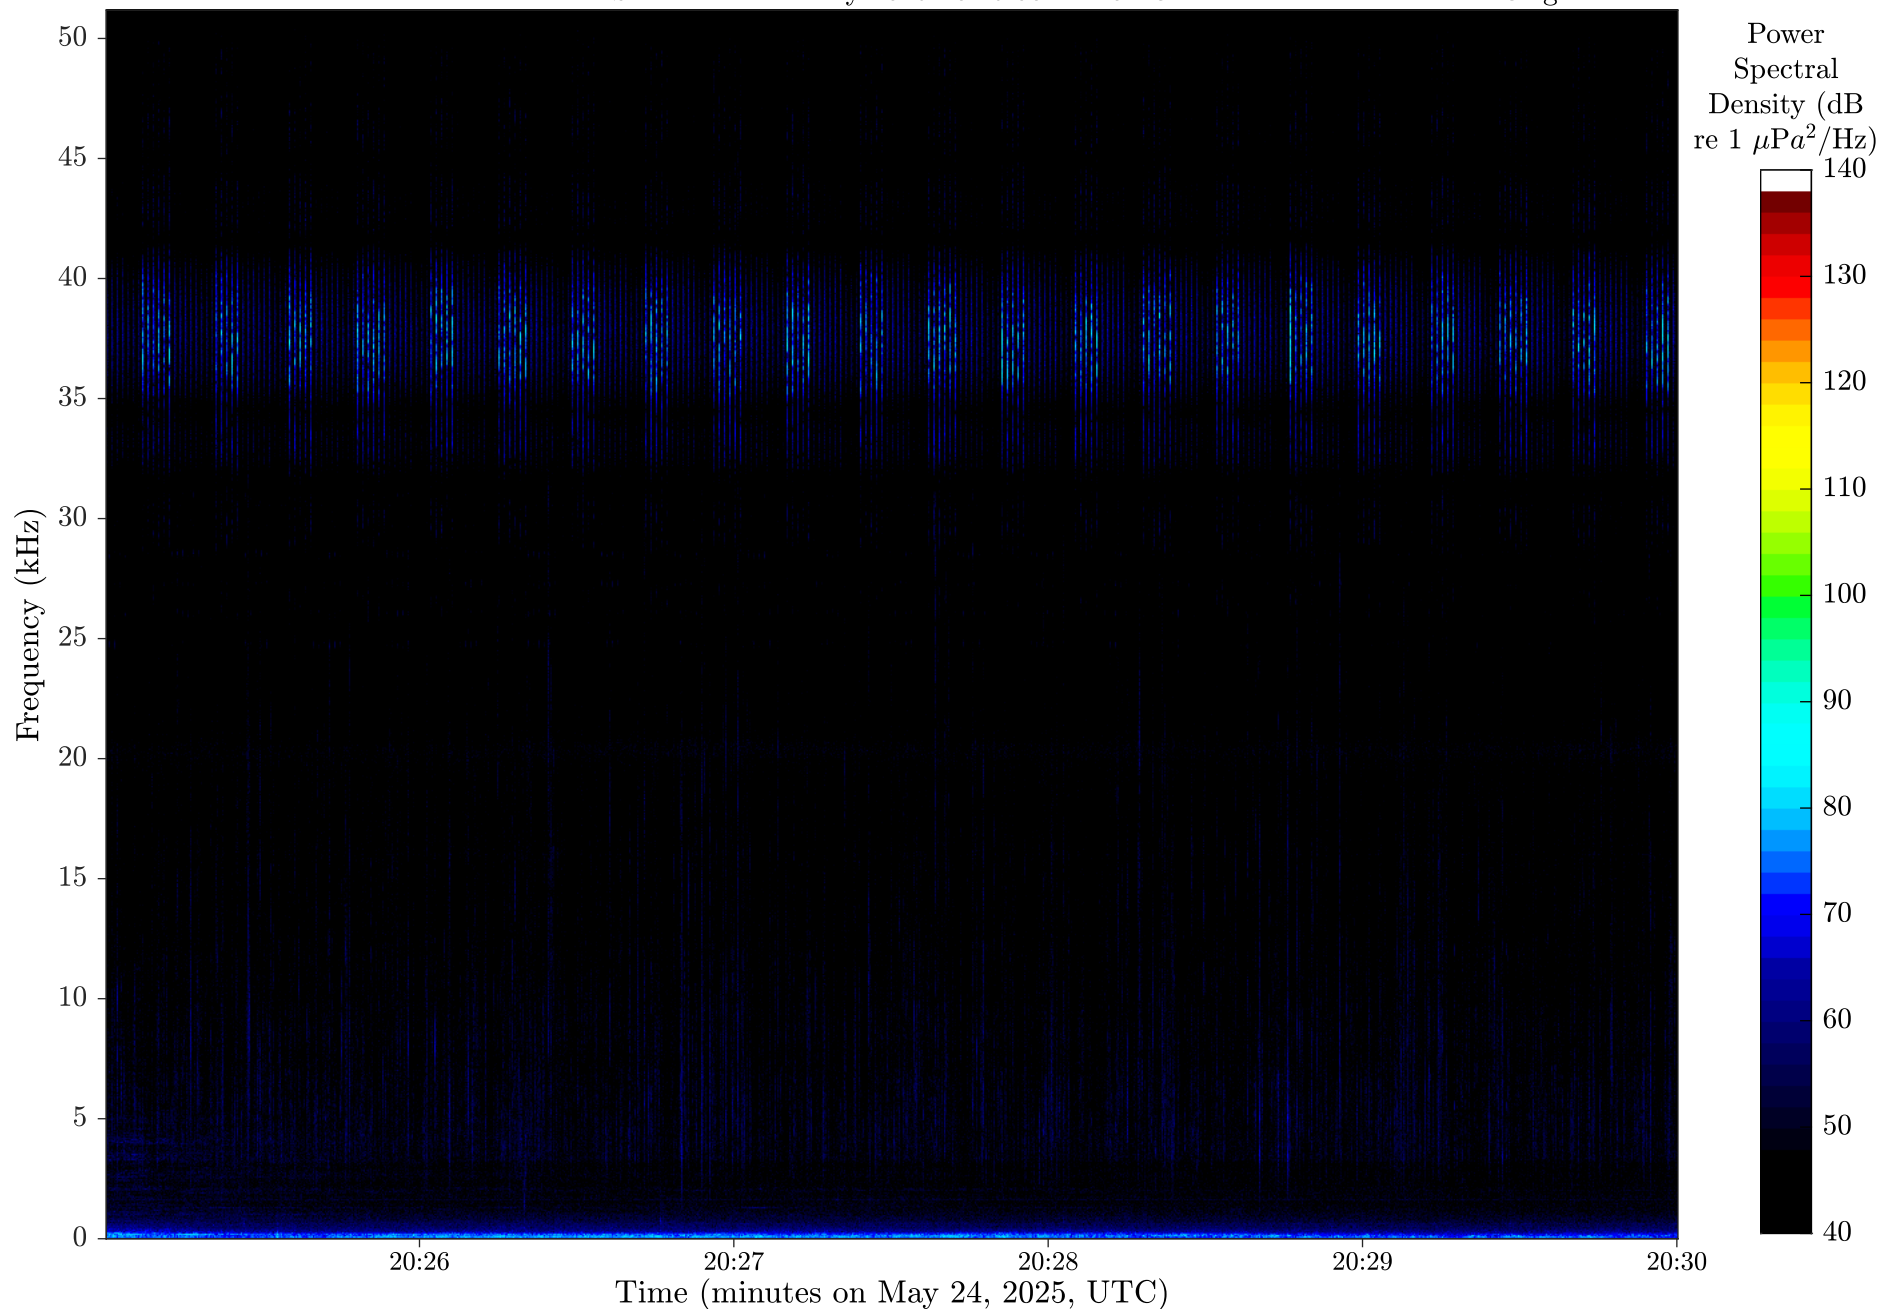


Comments: 34.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:52:21 UTC

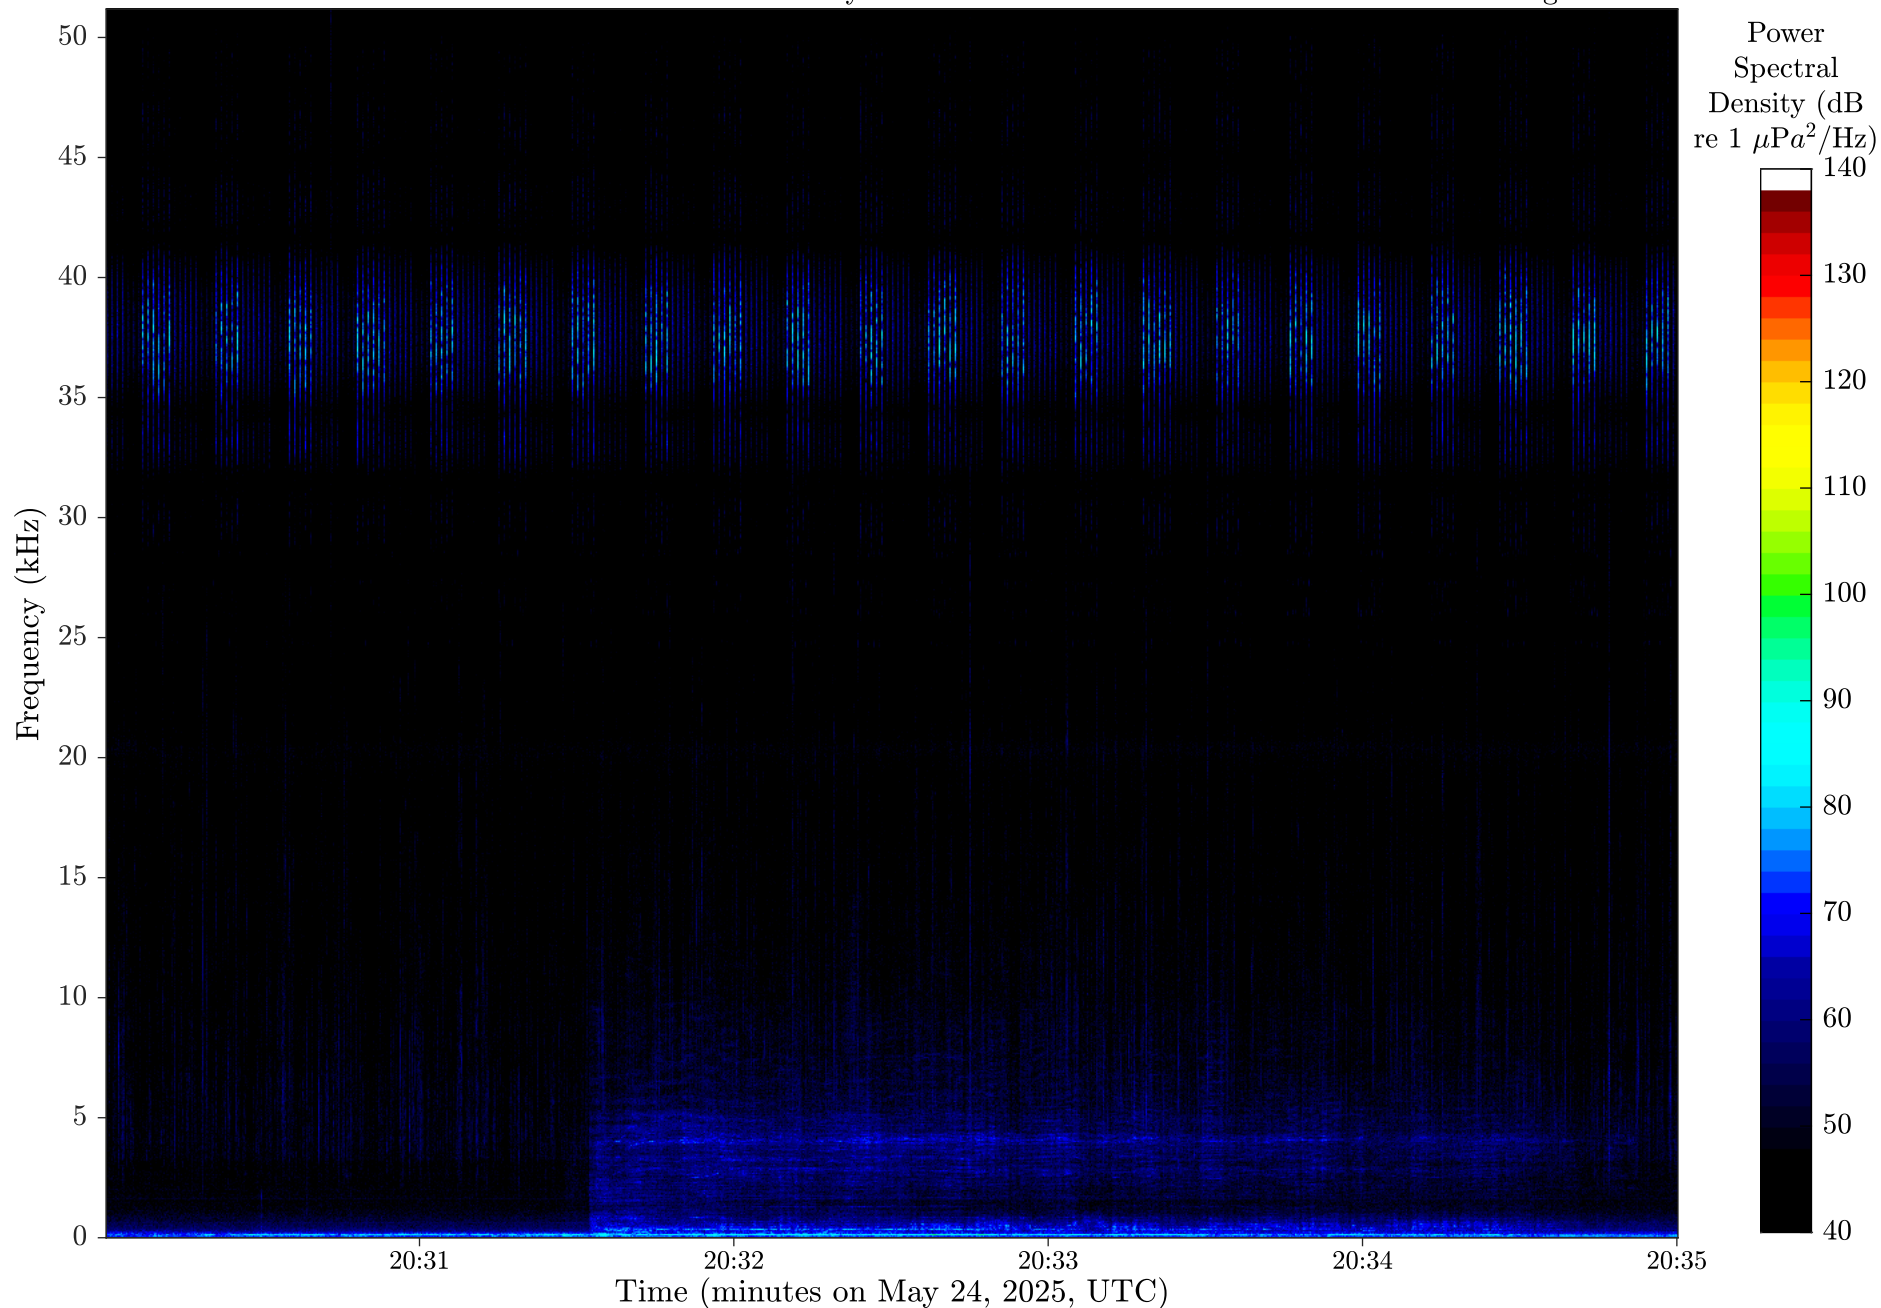


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:52:30 UTC

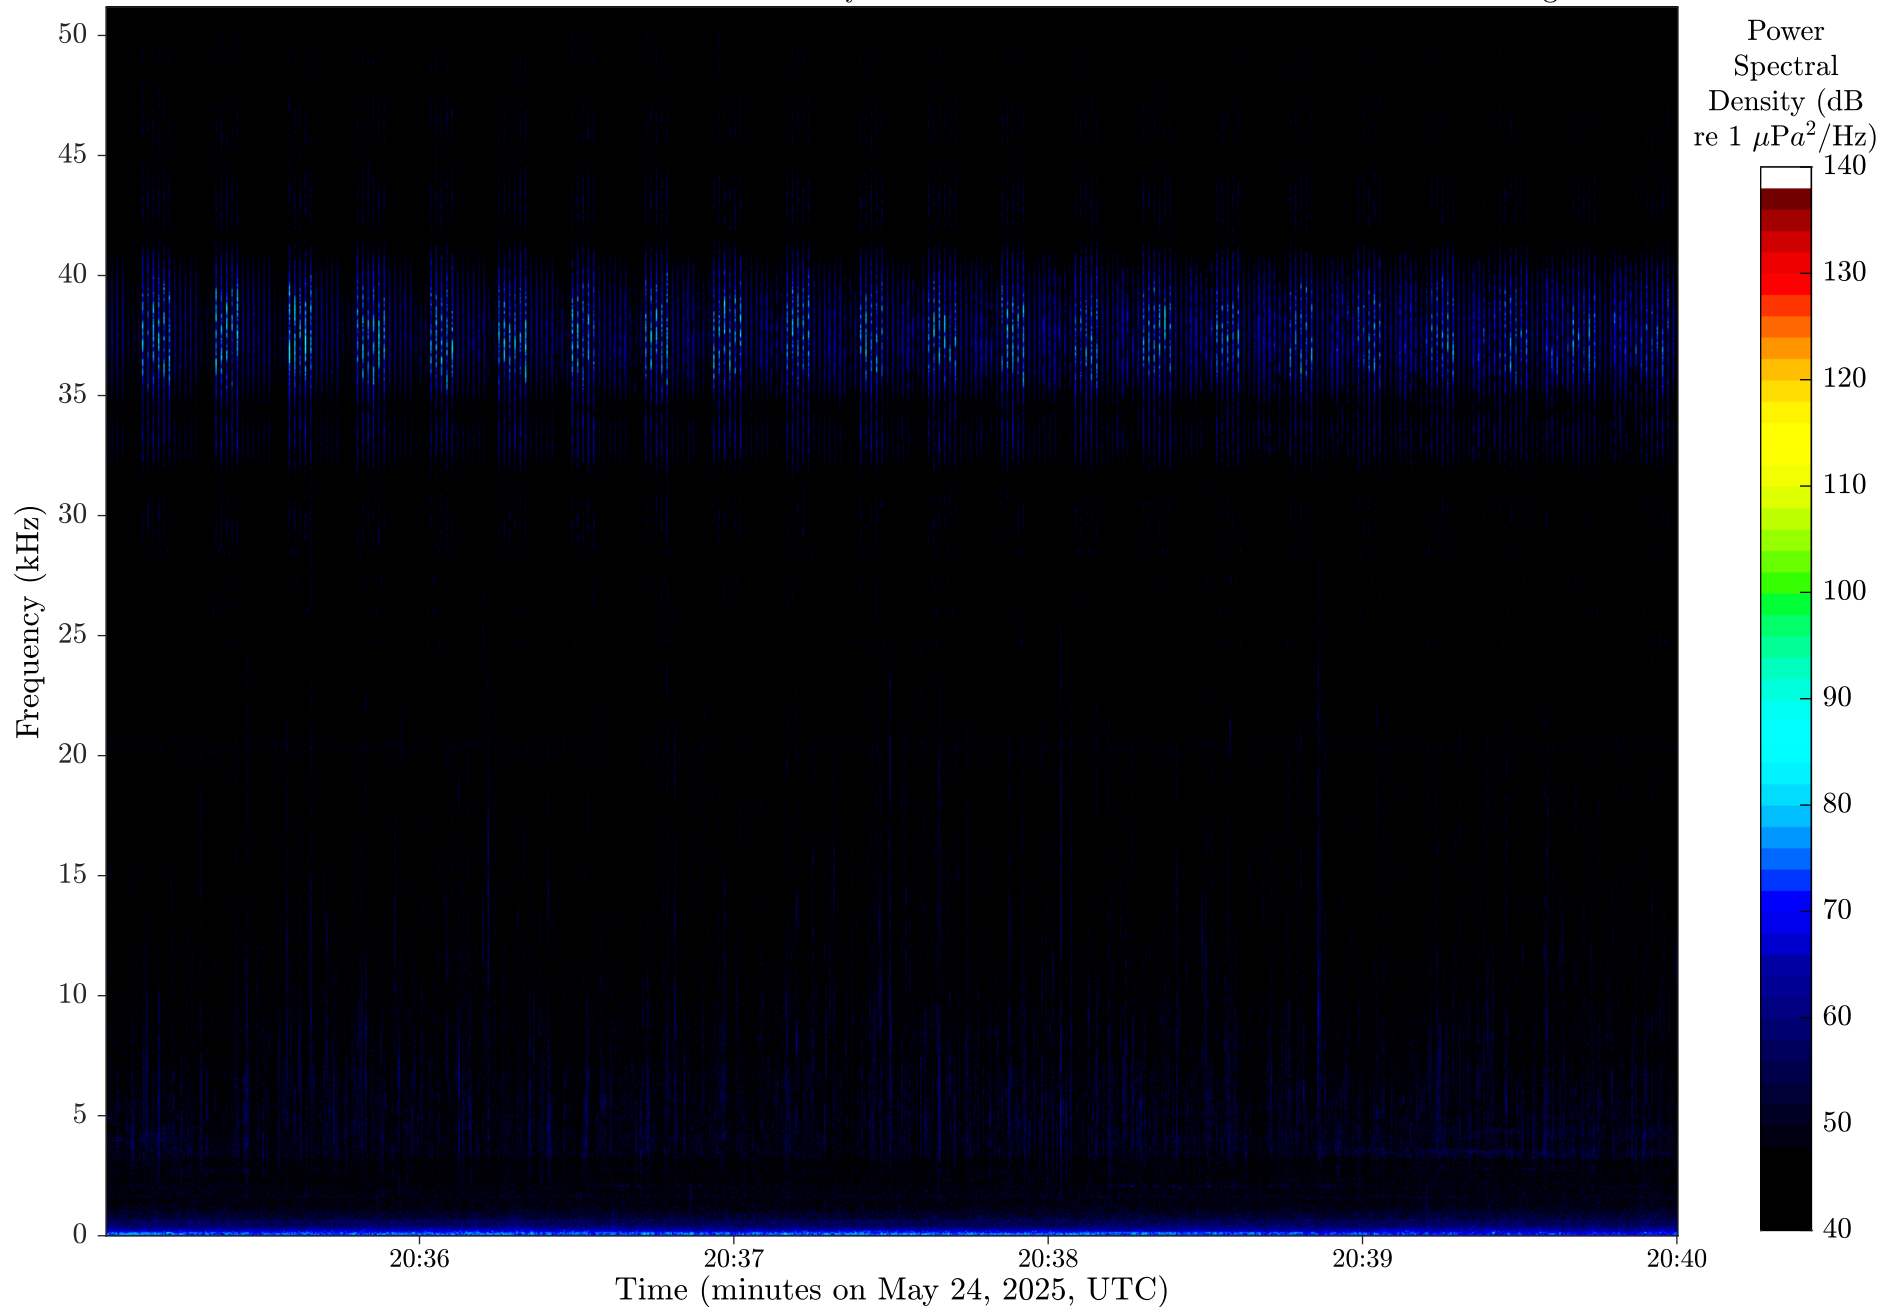


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:52:38 UTC

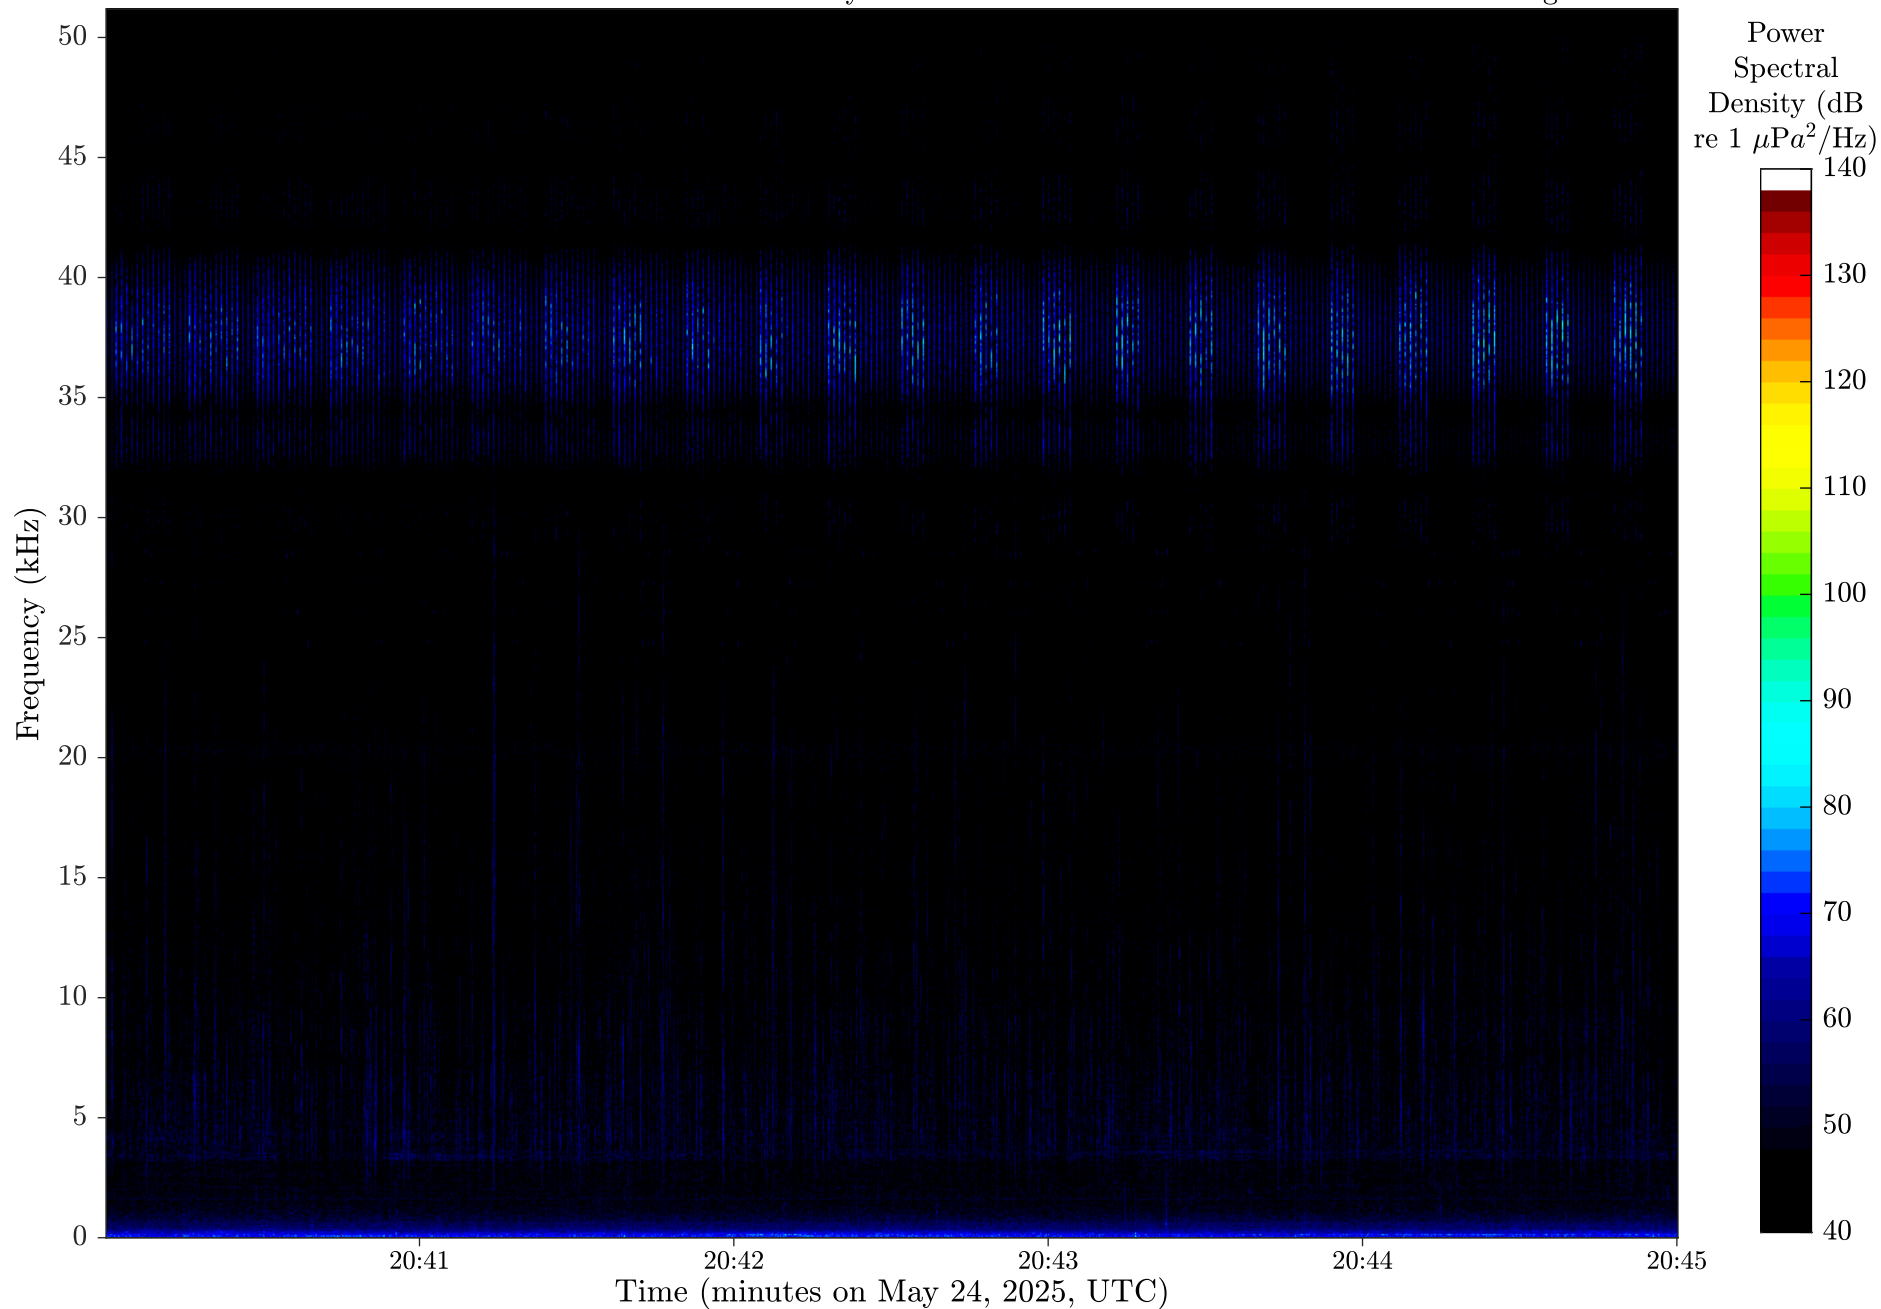


Comments: 32.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:52:47 UTC

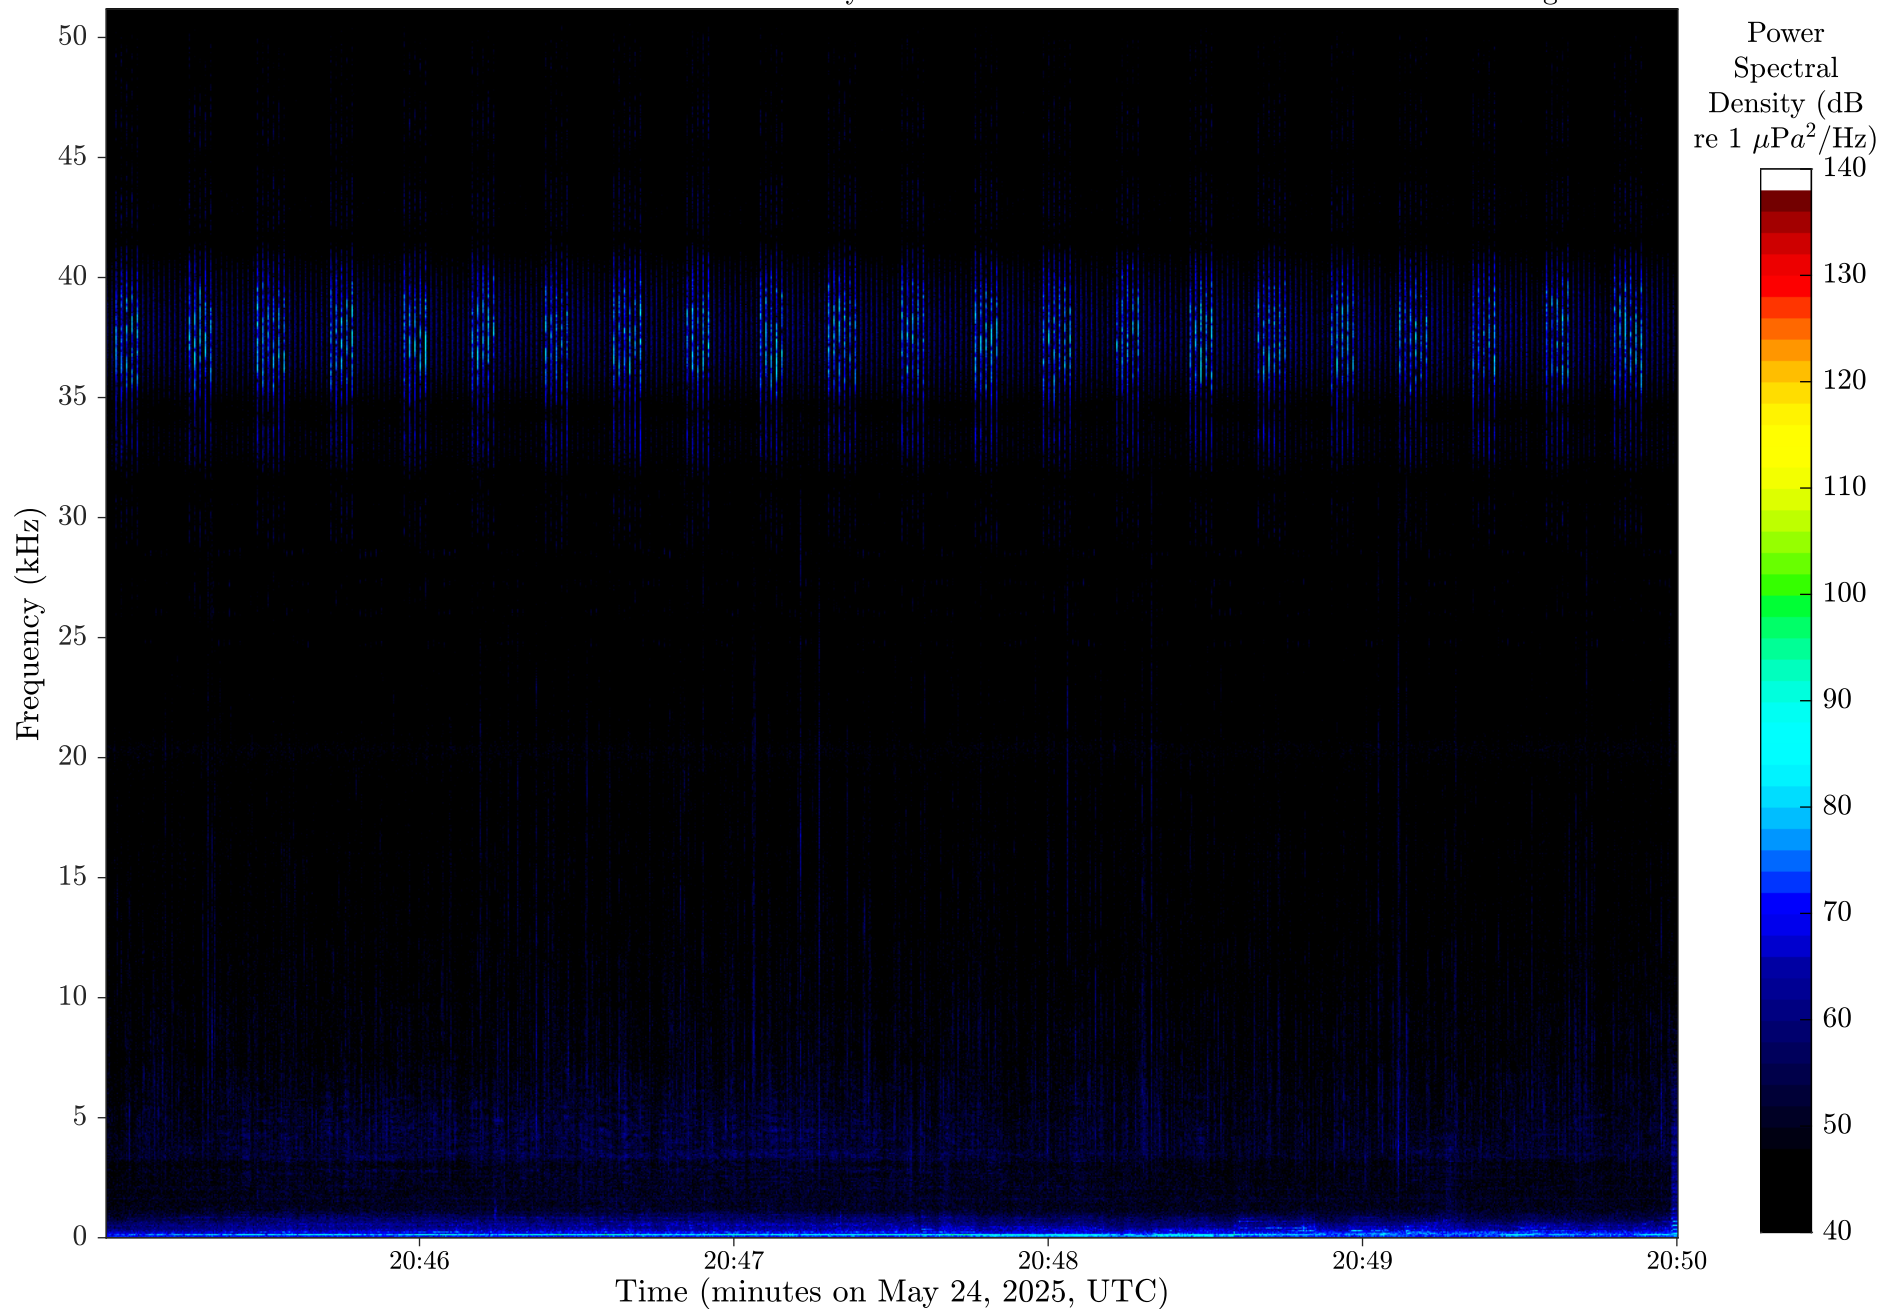


Comments: 33 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:52:55 UTC

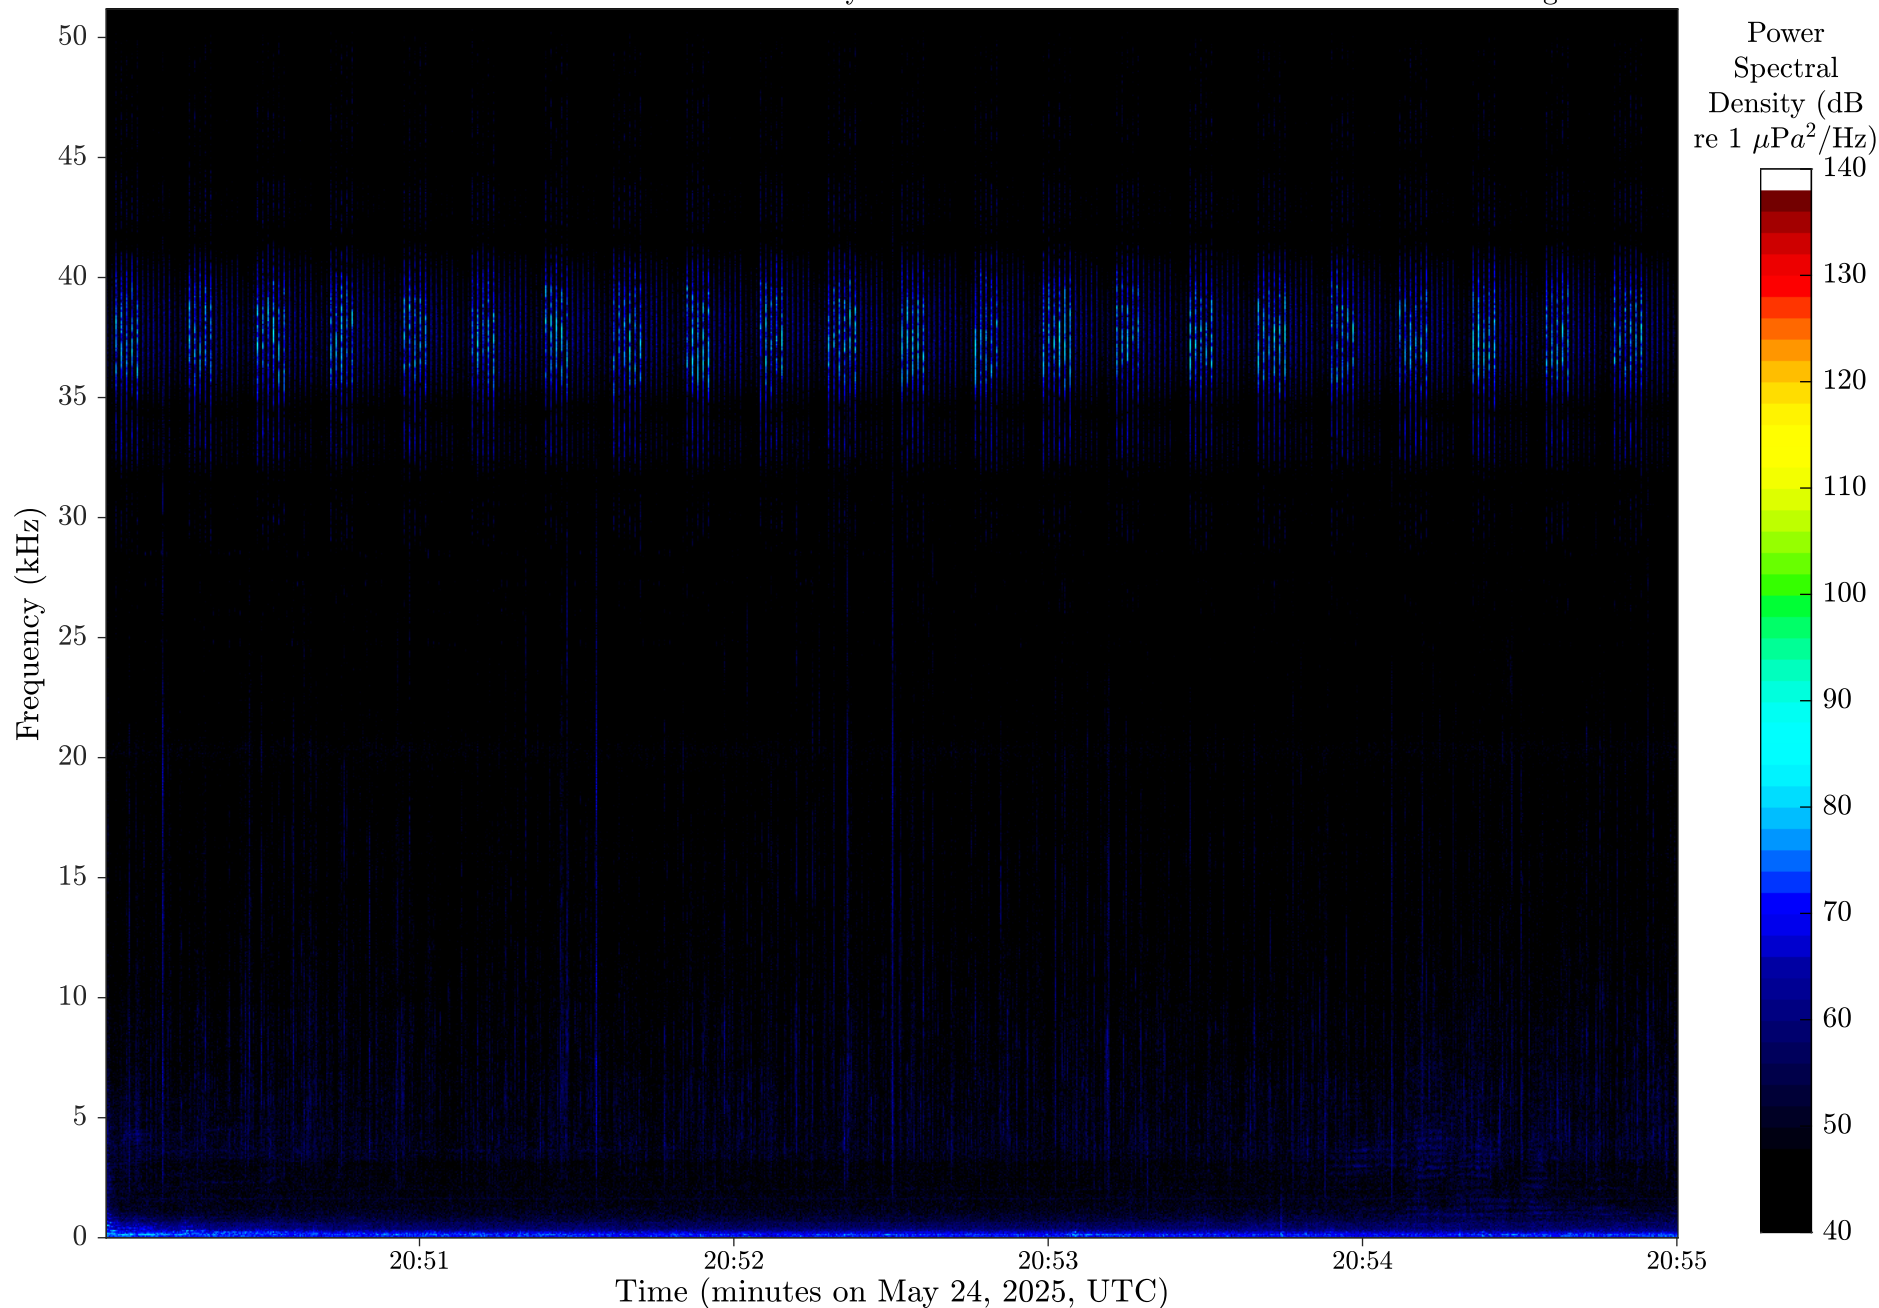


Comments: 33.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:53:04 UTC

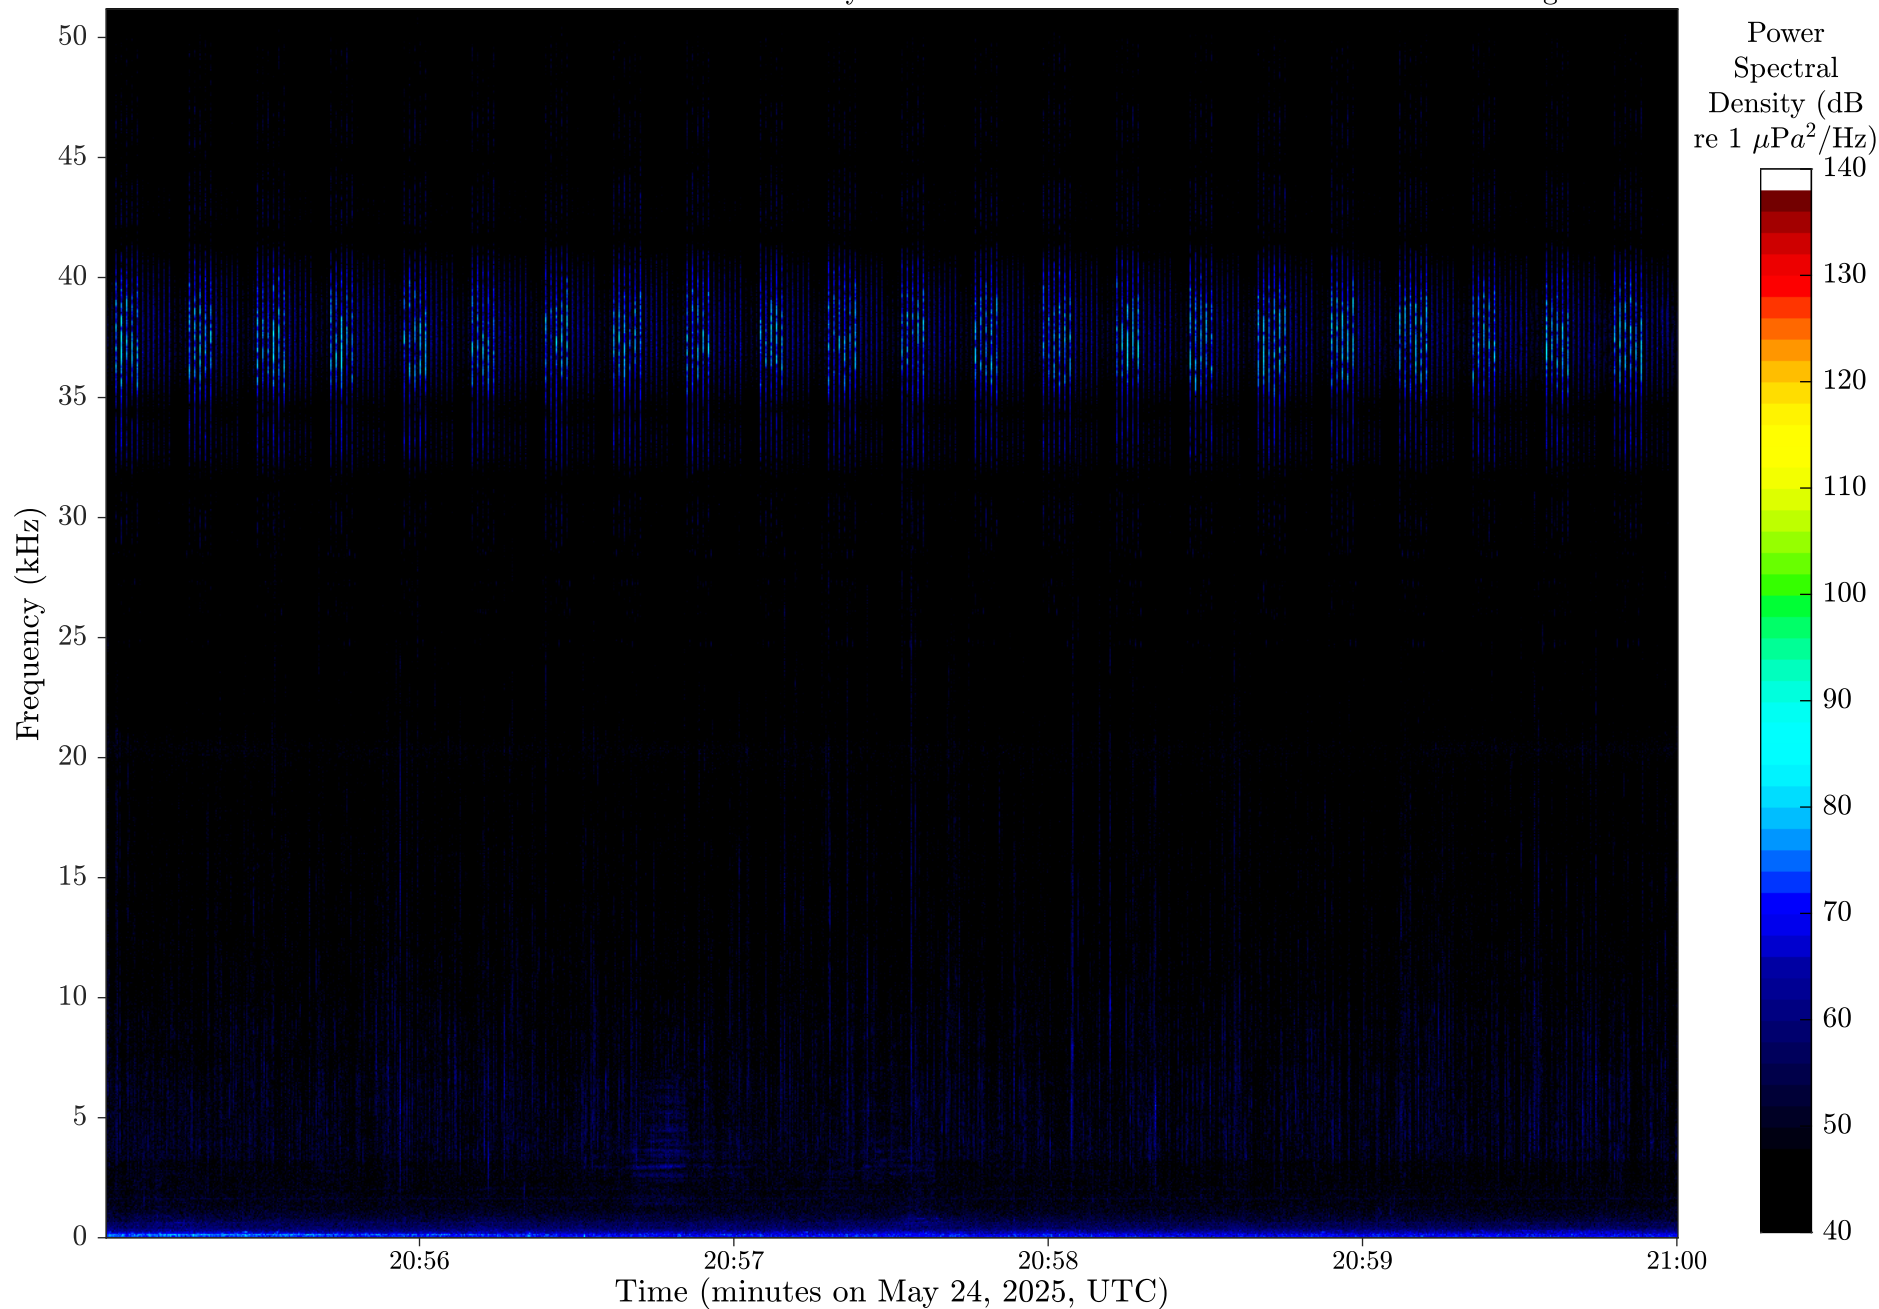


Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:53:11 UTC

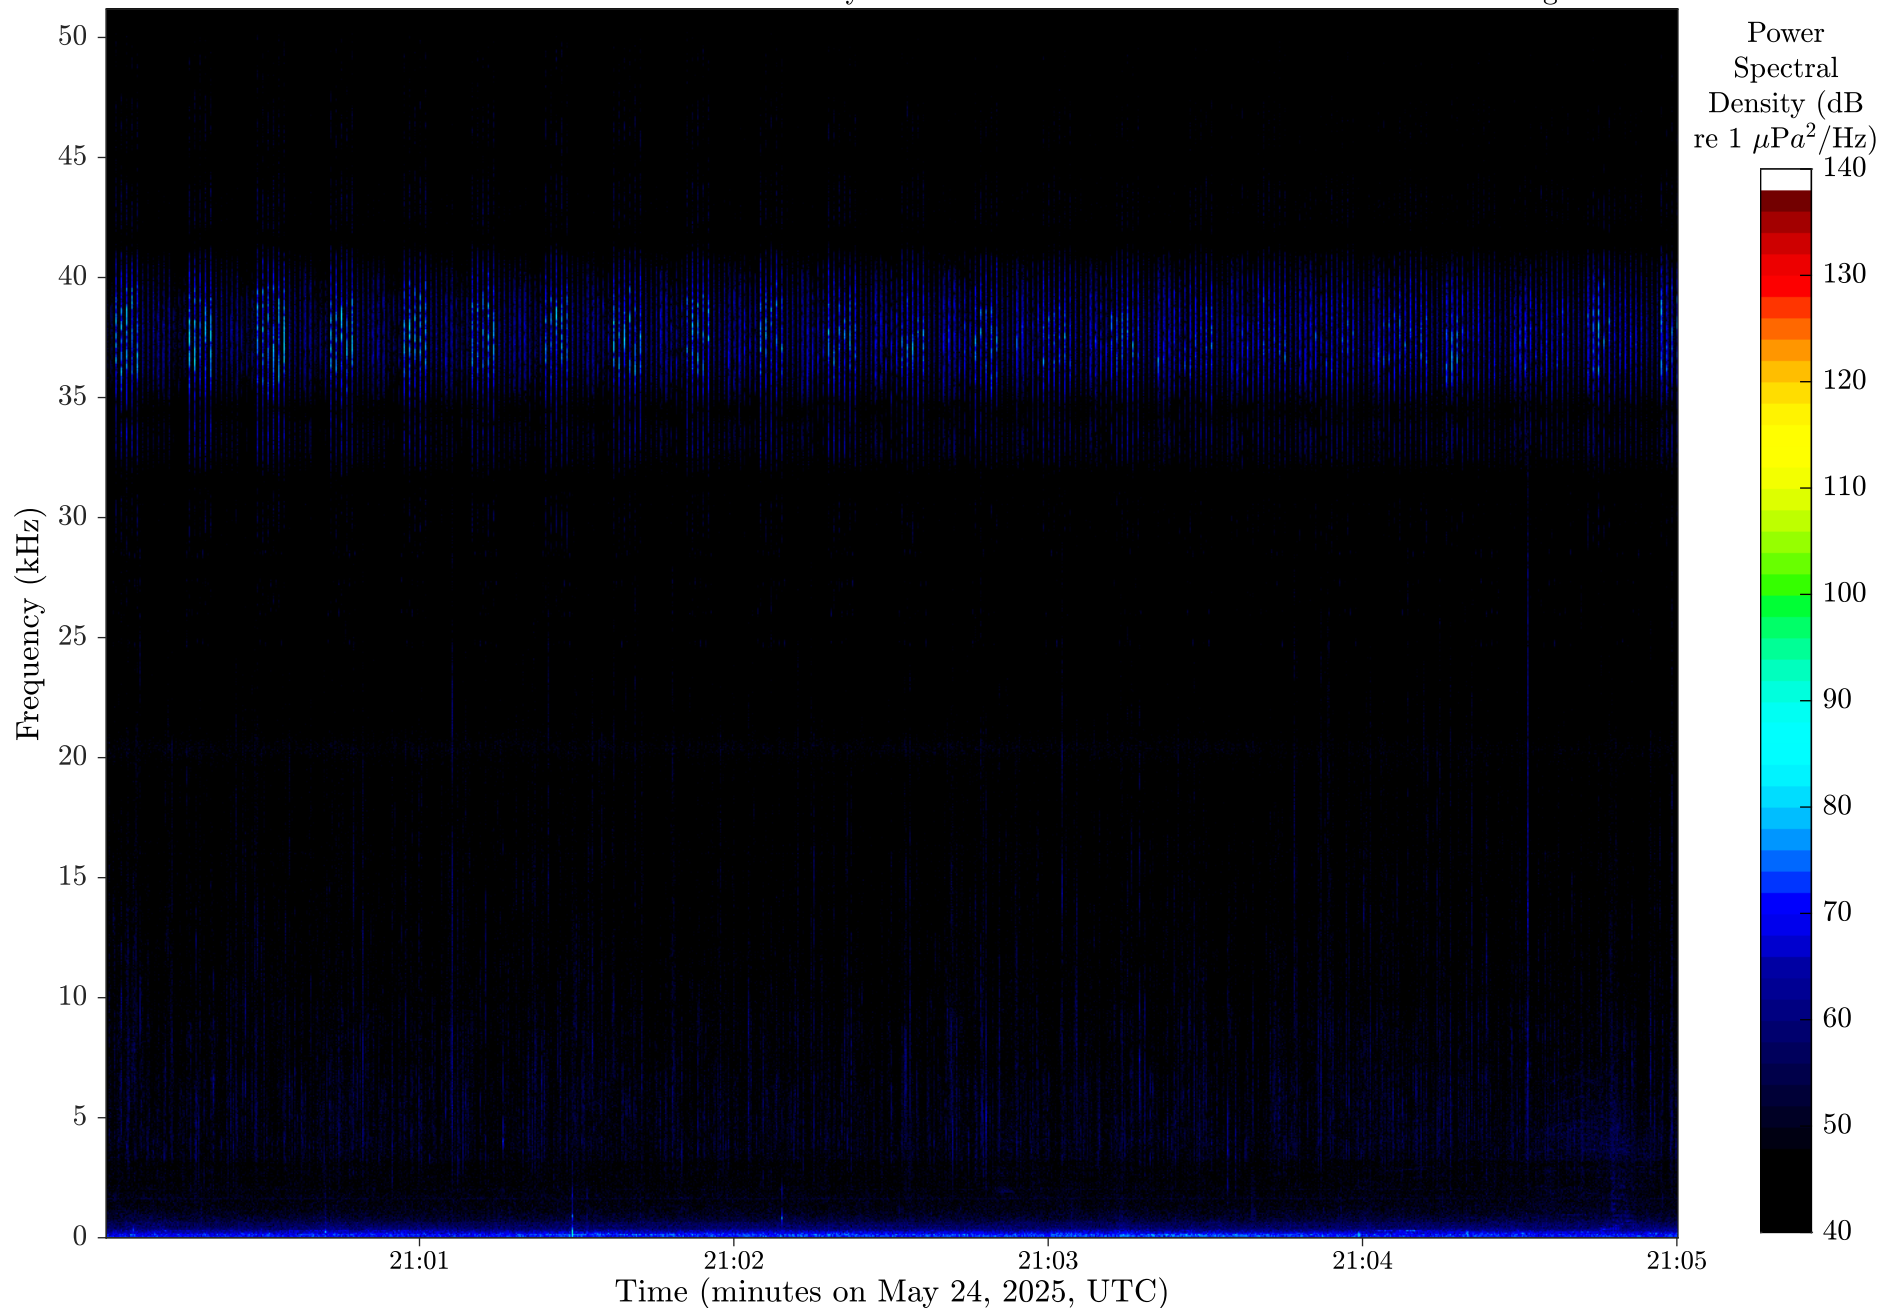


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:53:20 UTC

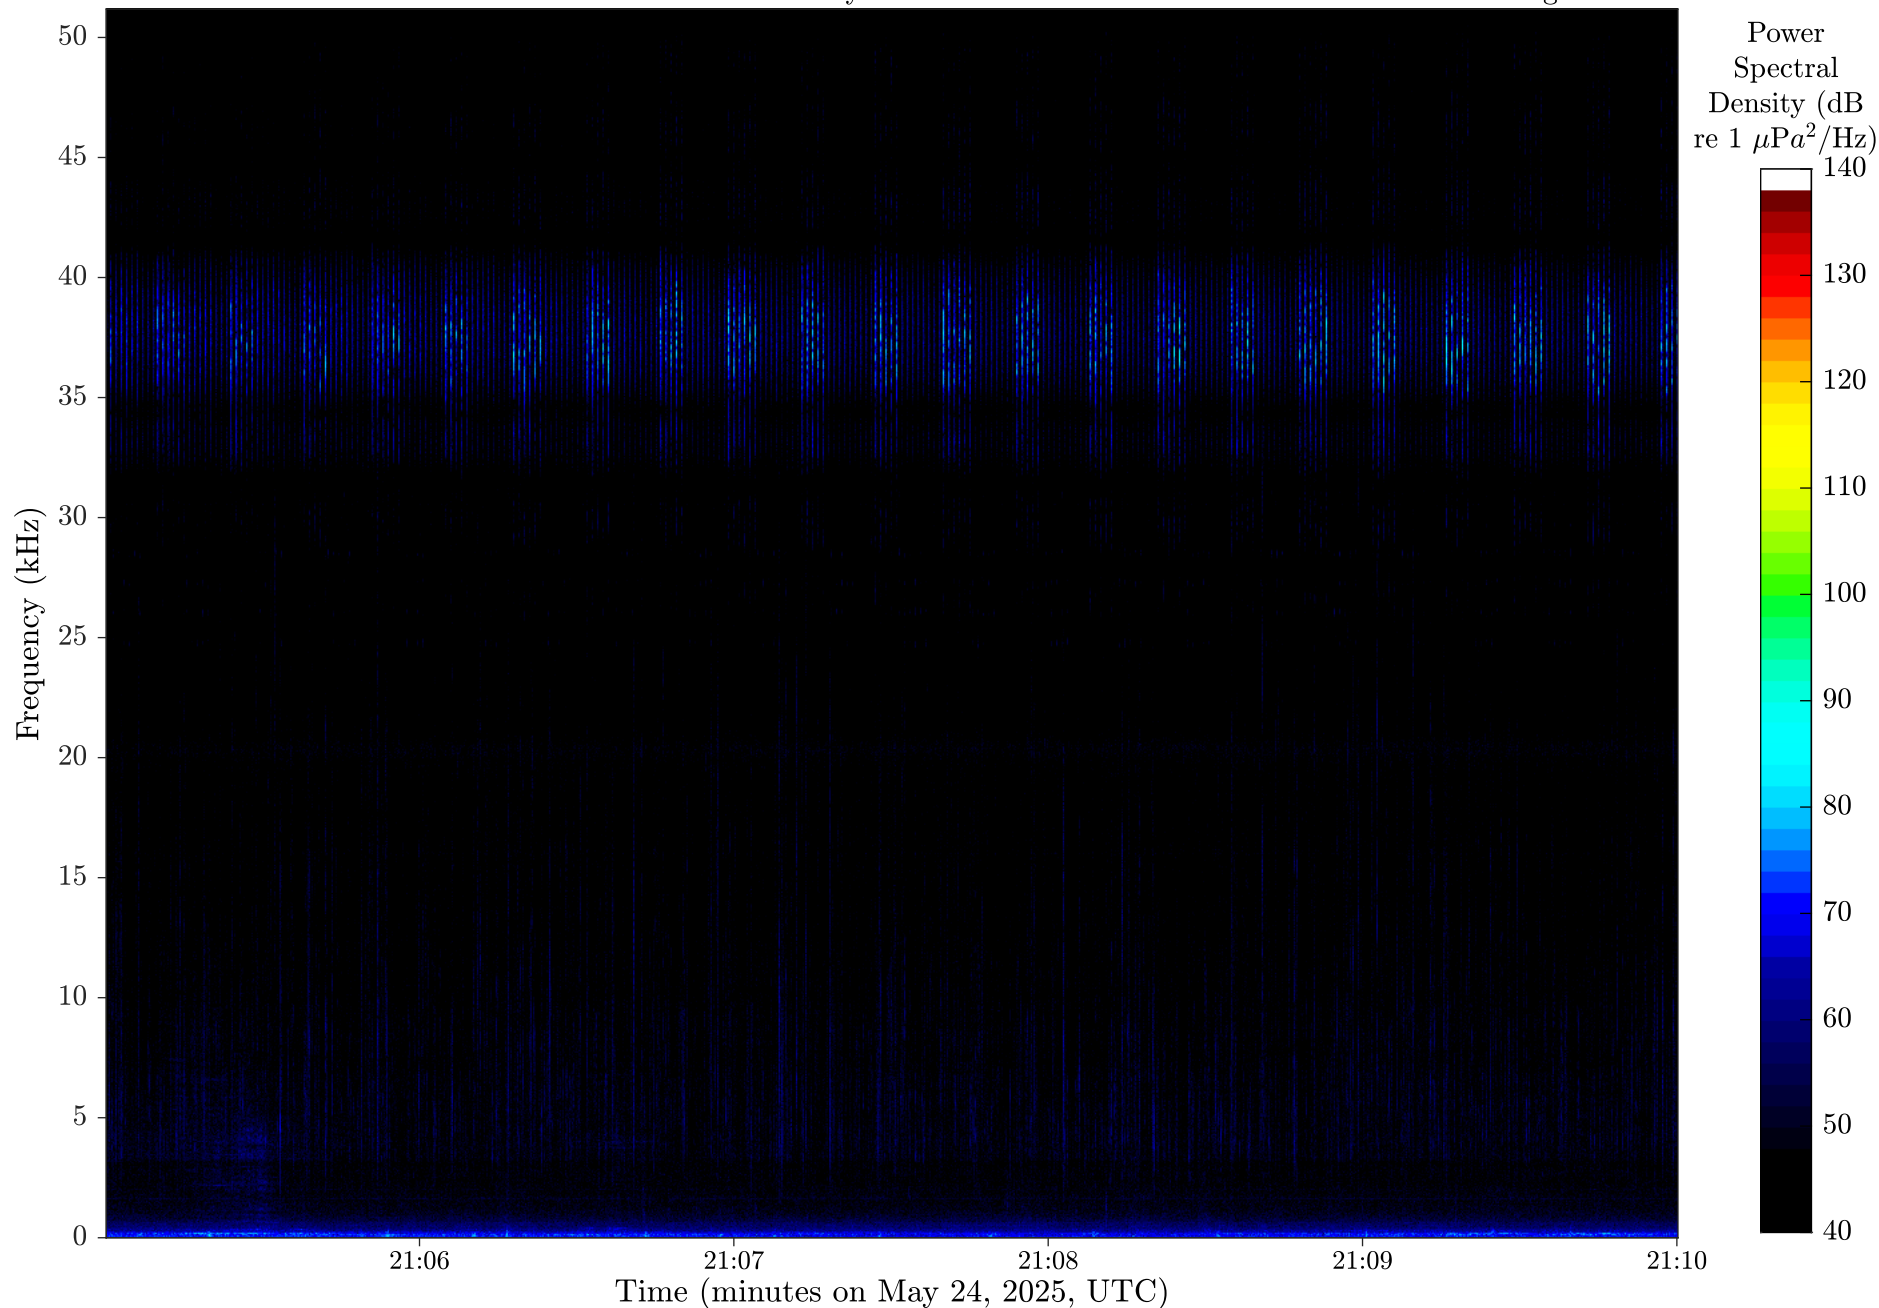


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:53:28 UTC

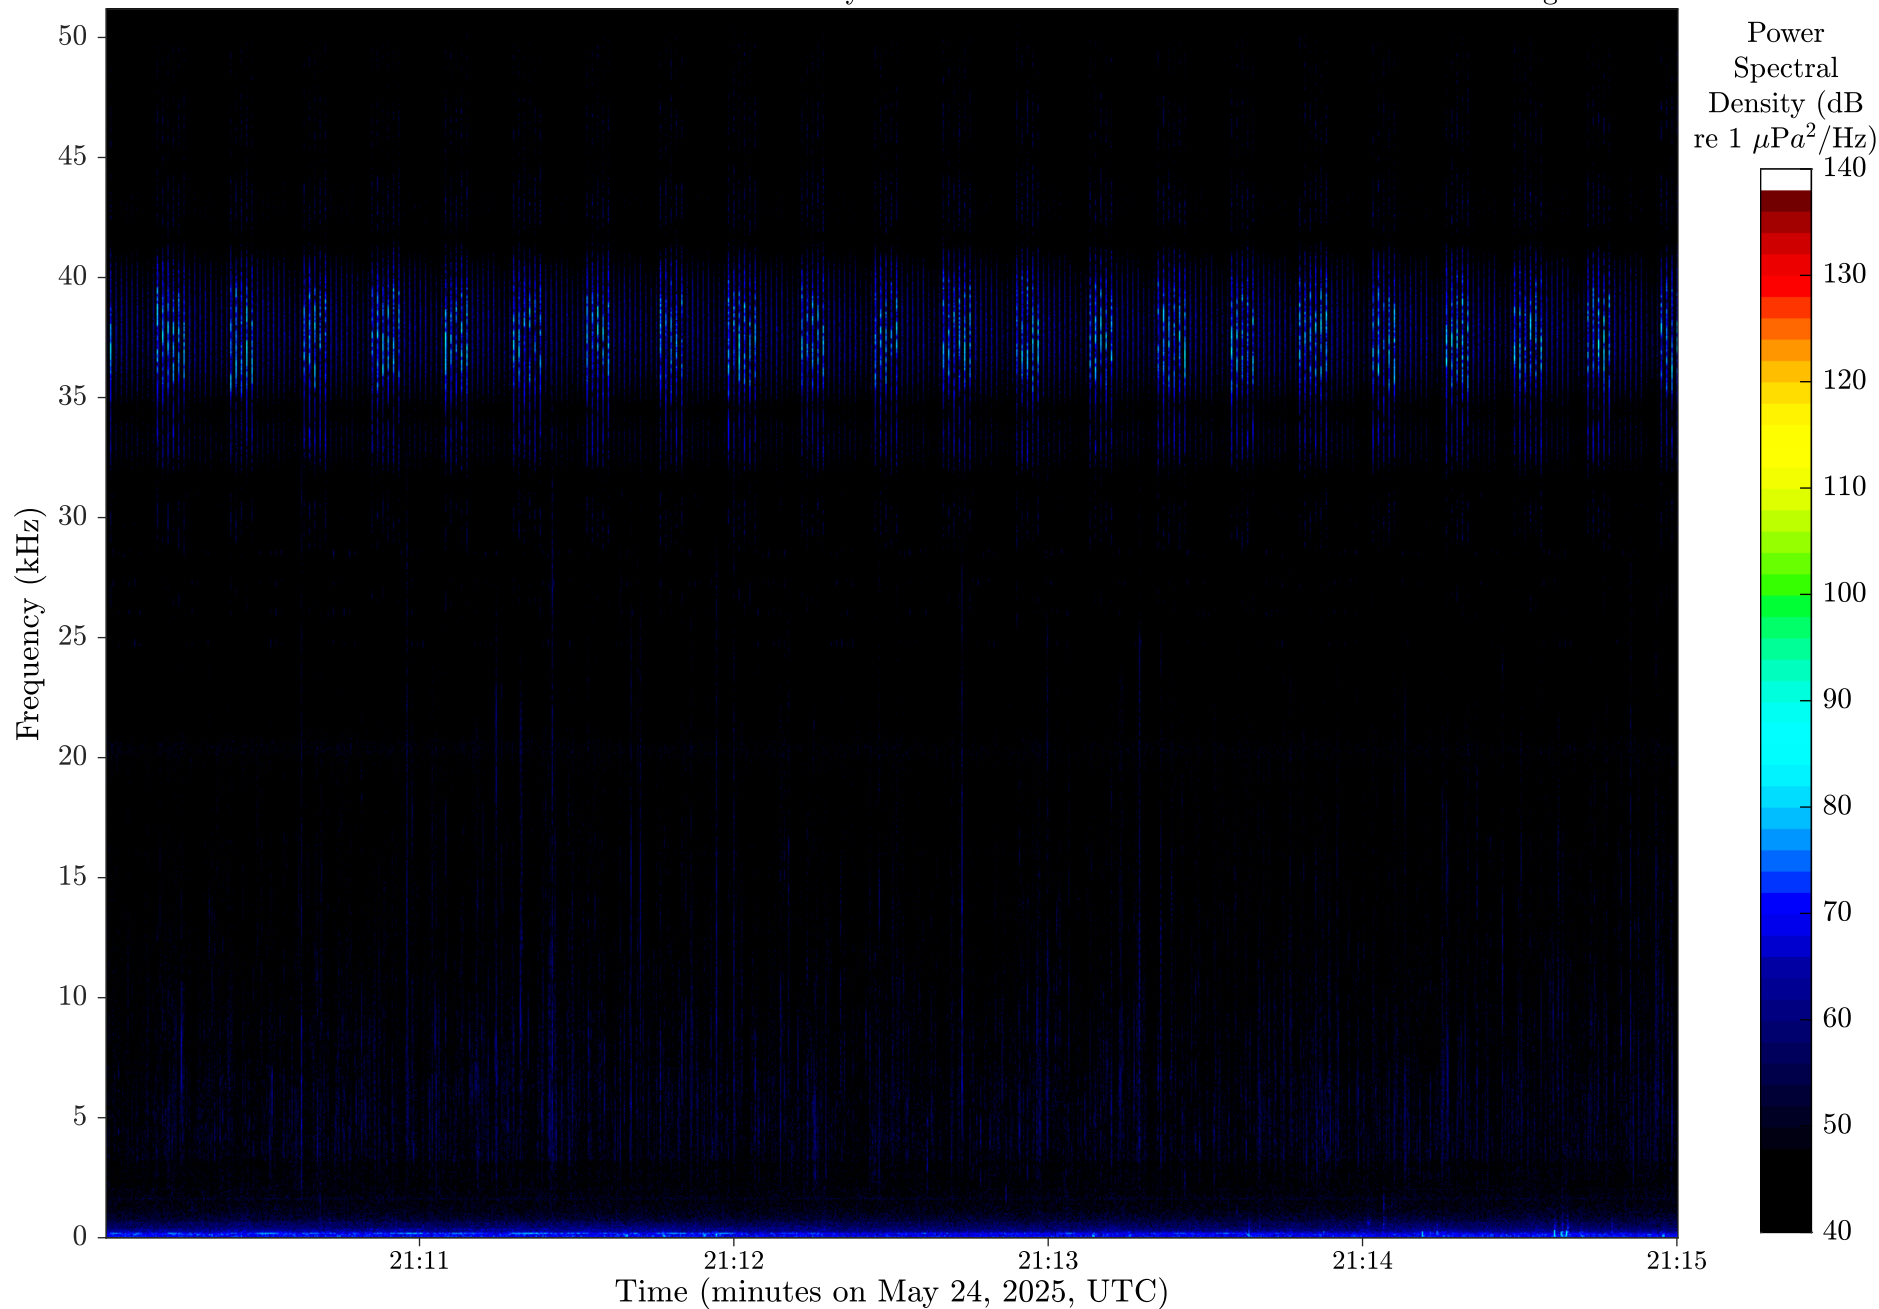


Comments: 34 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:53:36 UTC

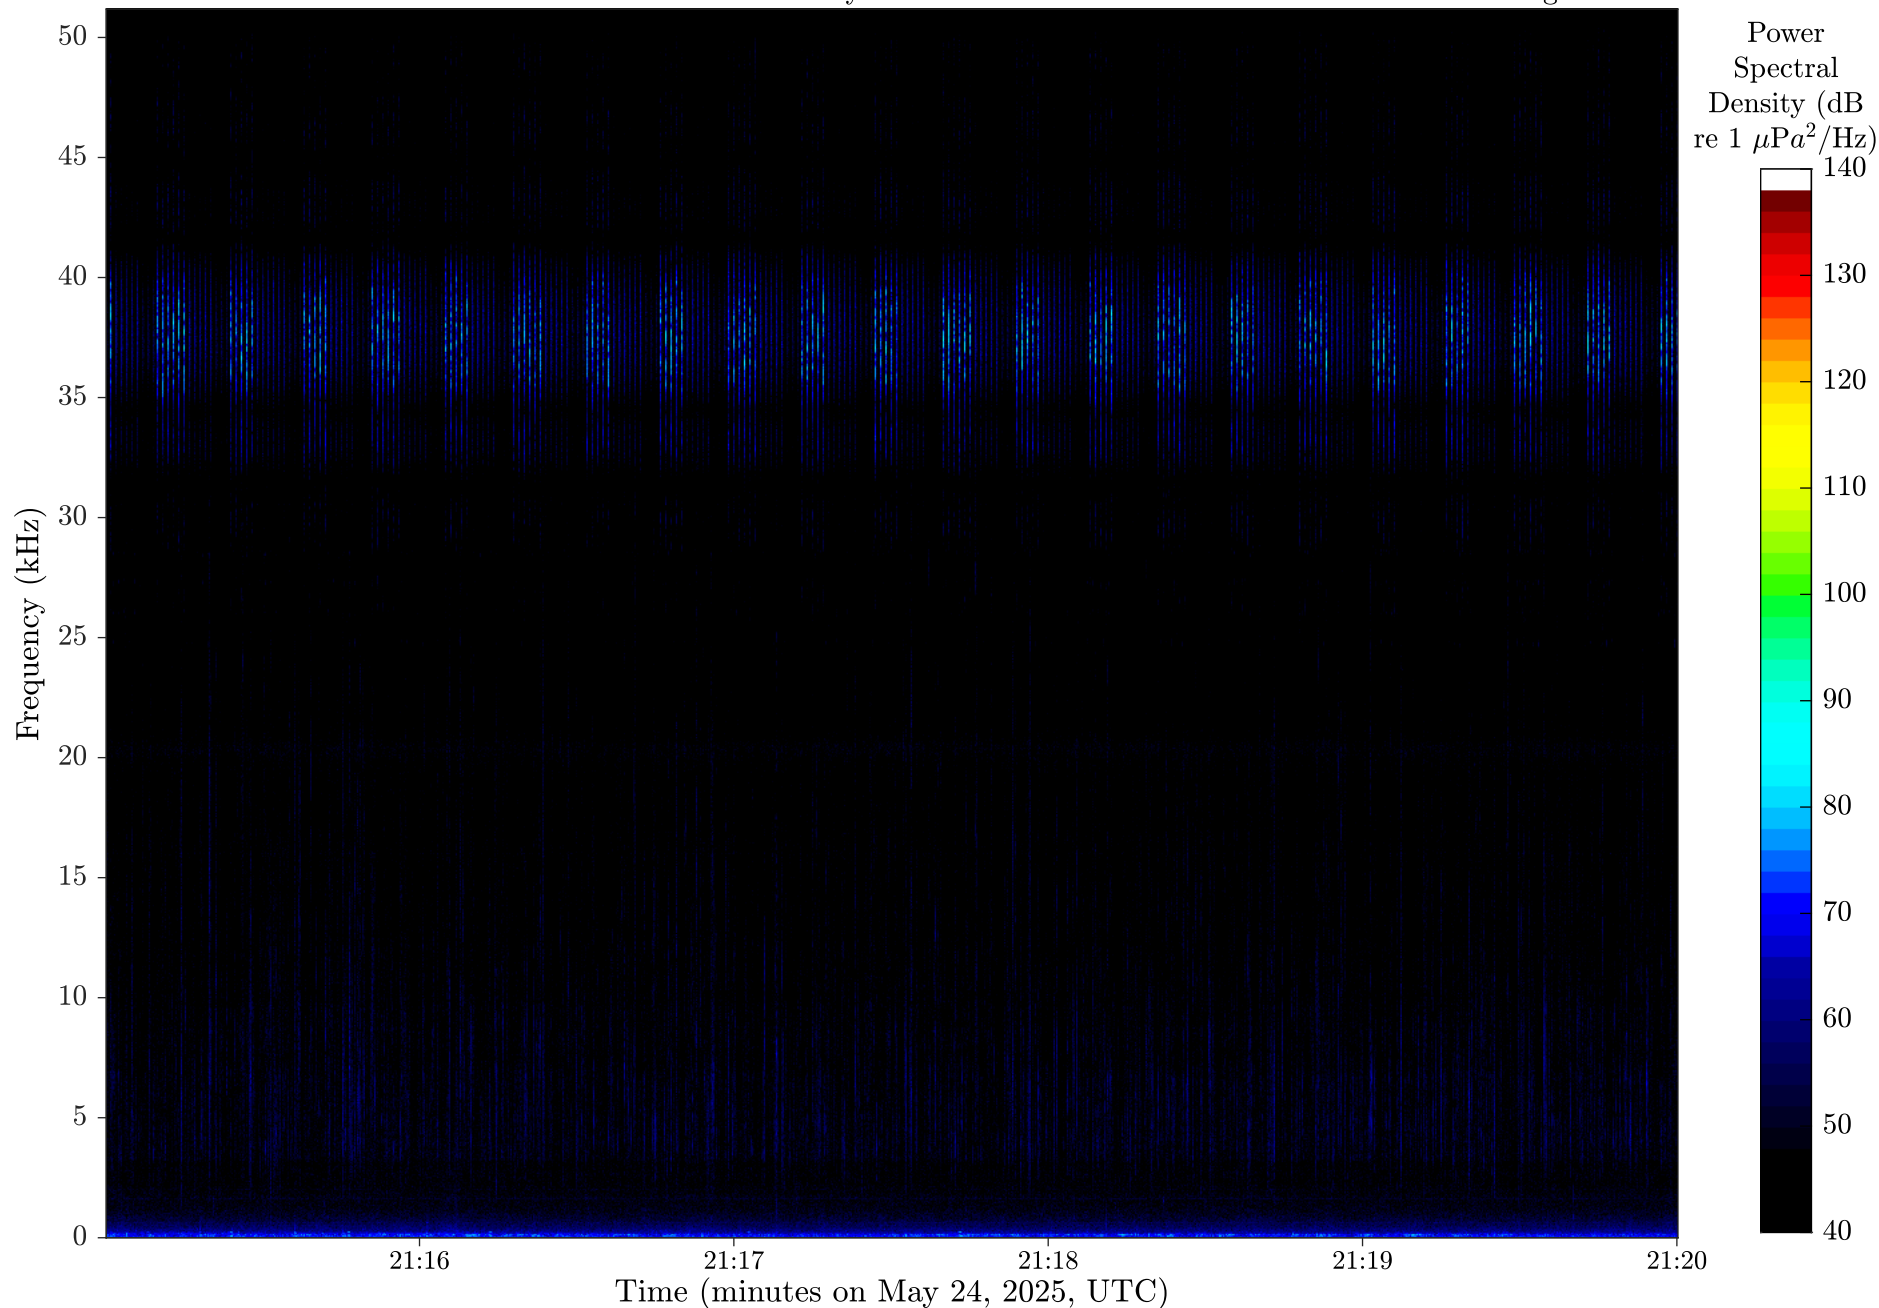


Comments: 34.4 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:53:44 UTC

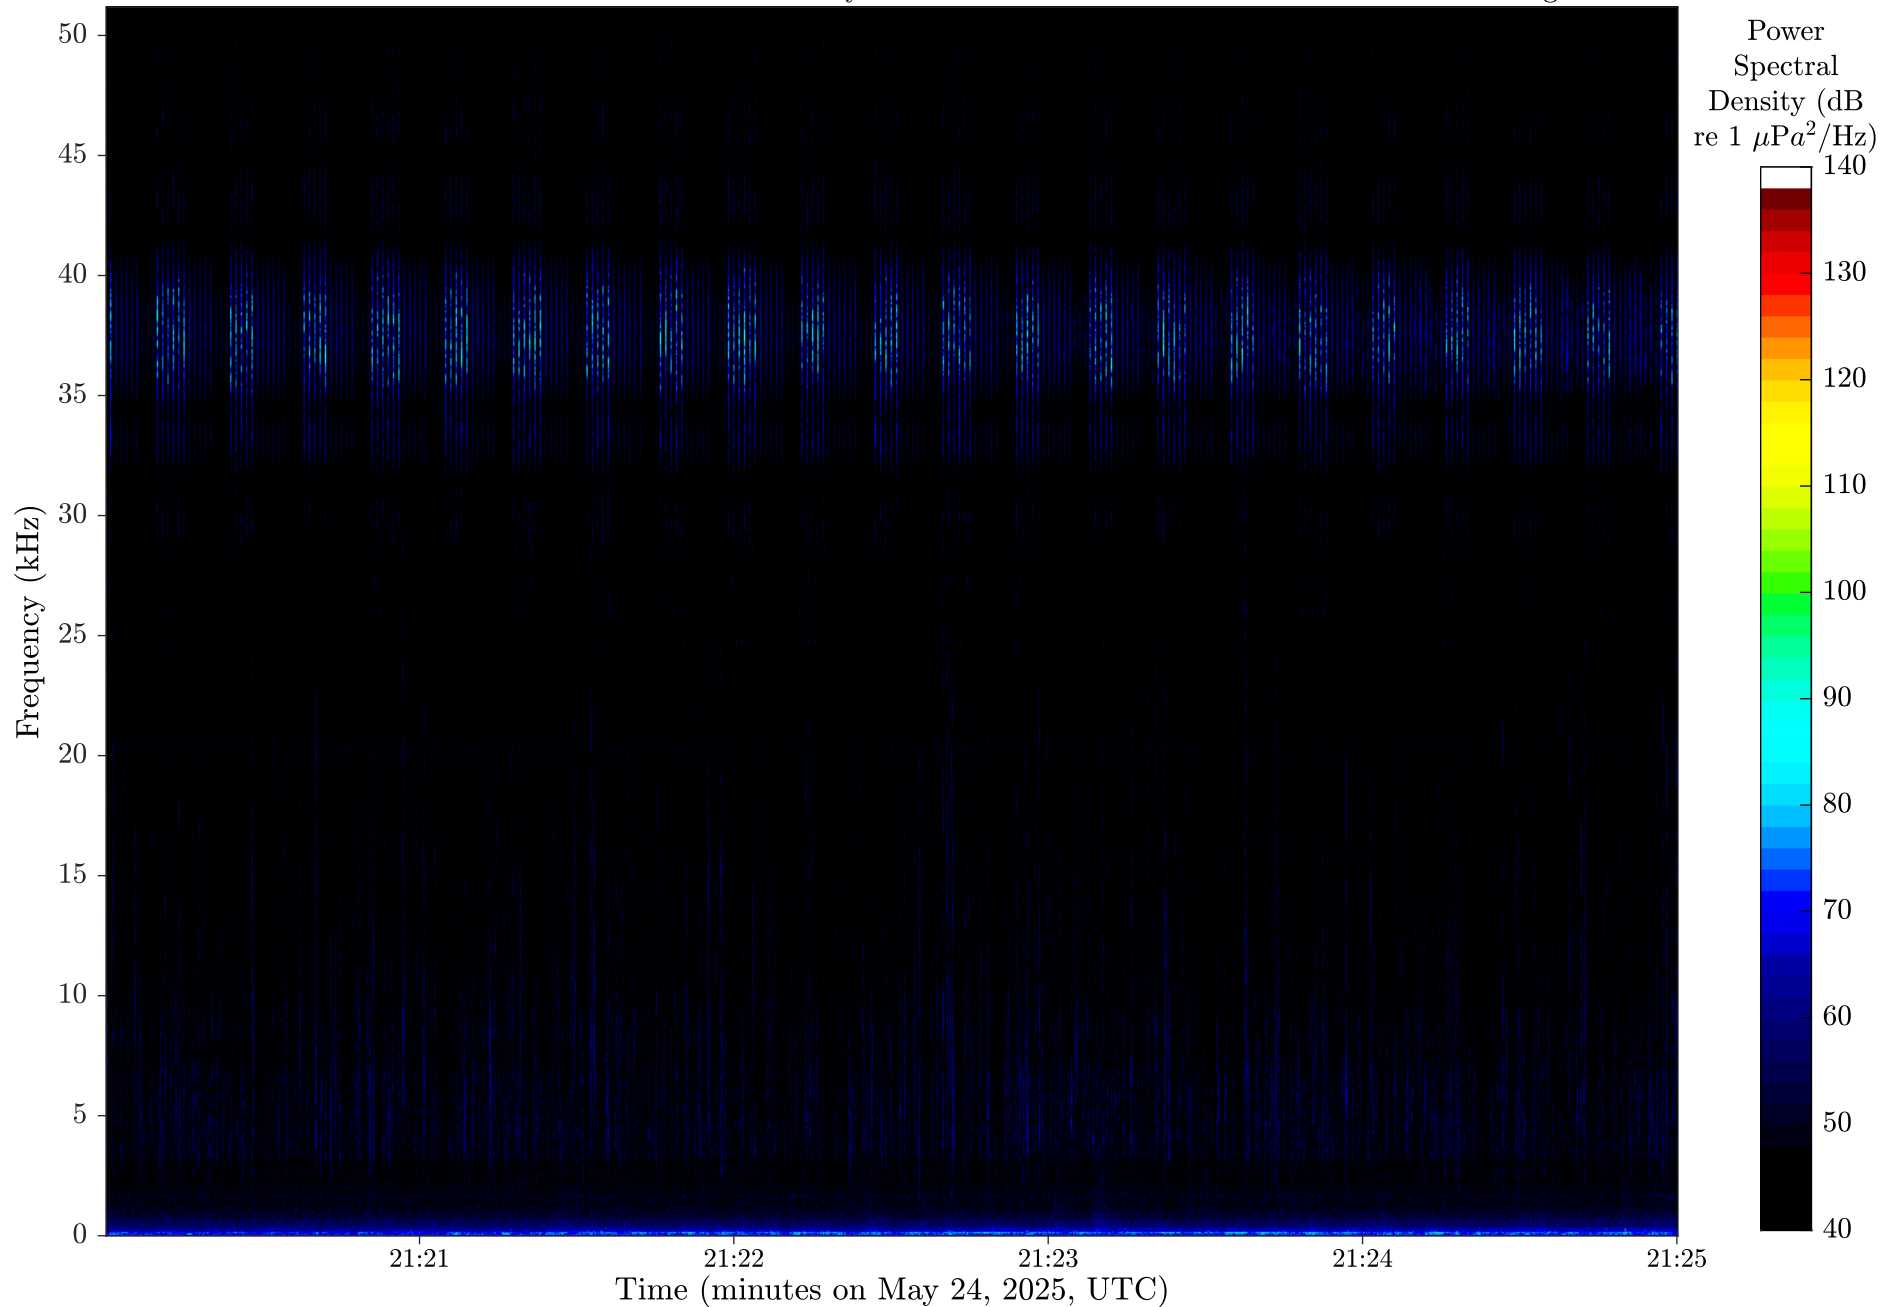


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:53:51 UTC

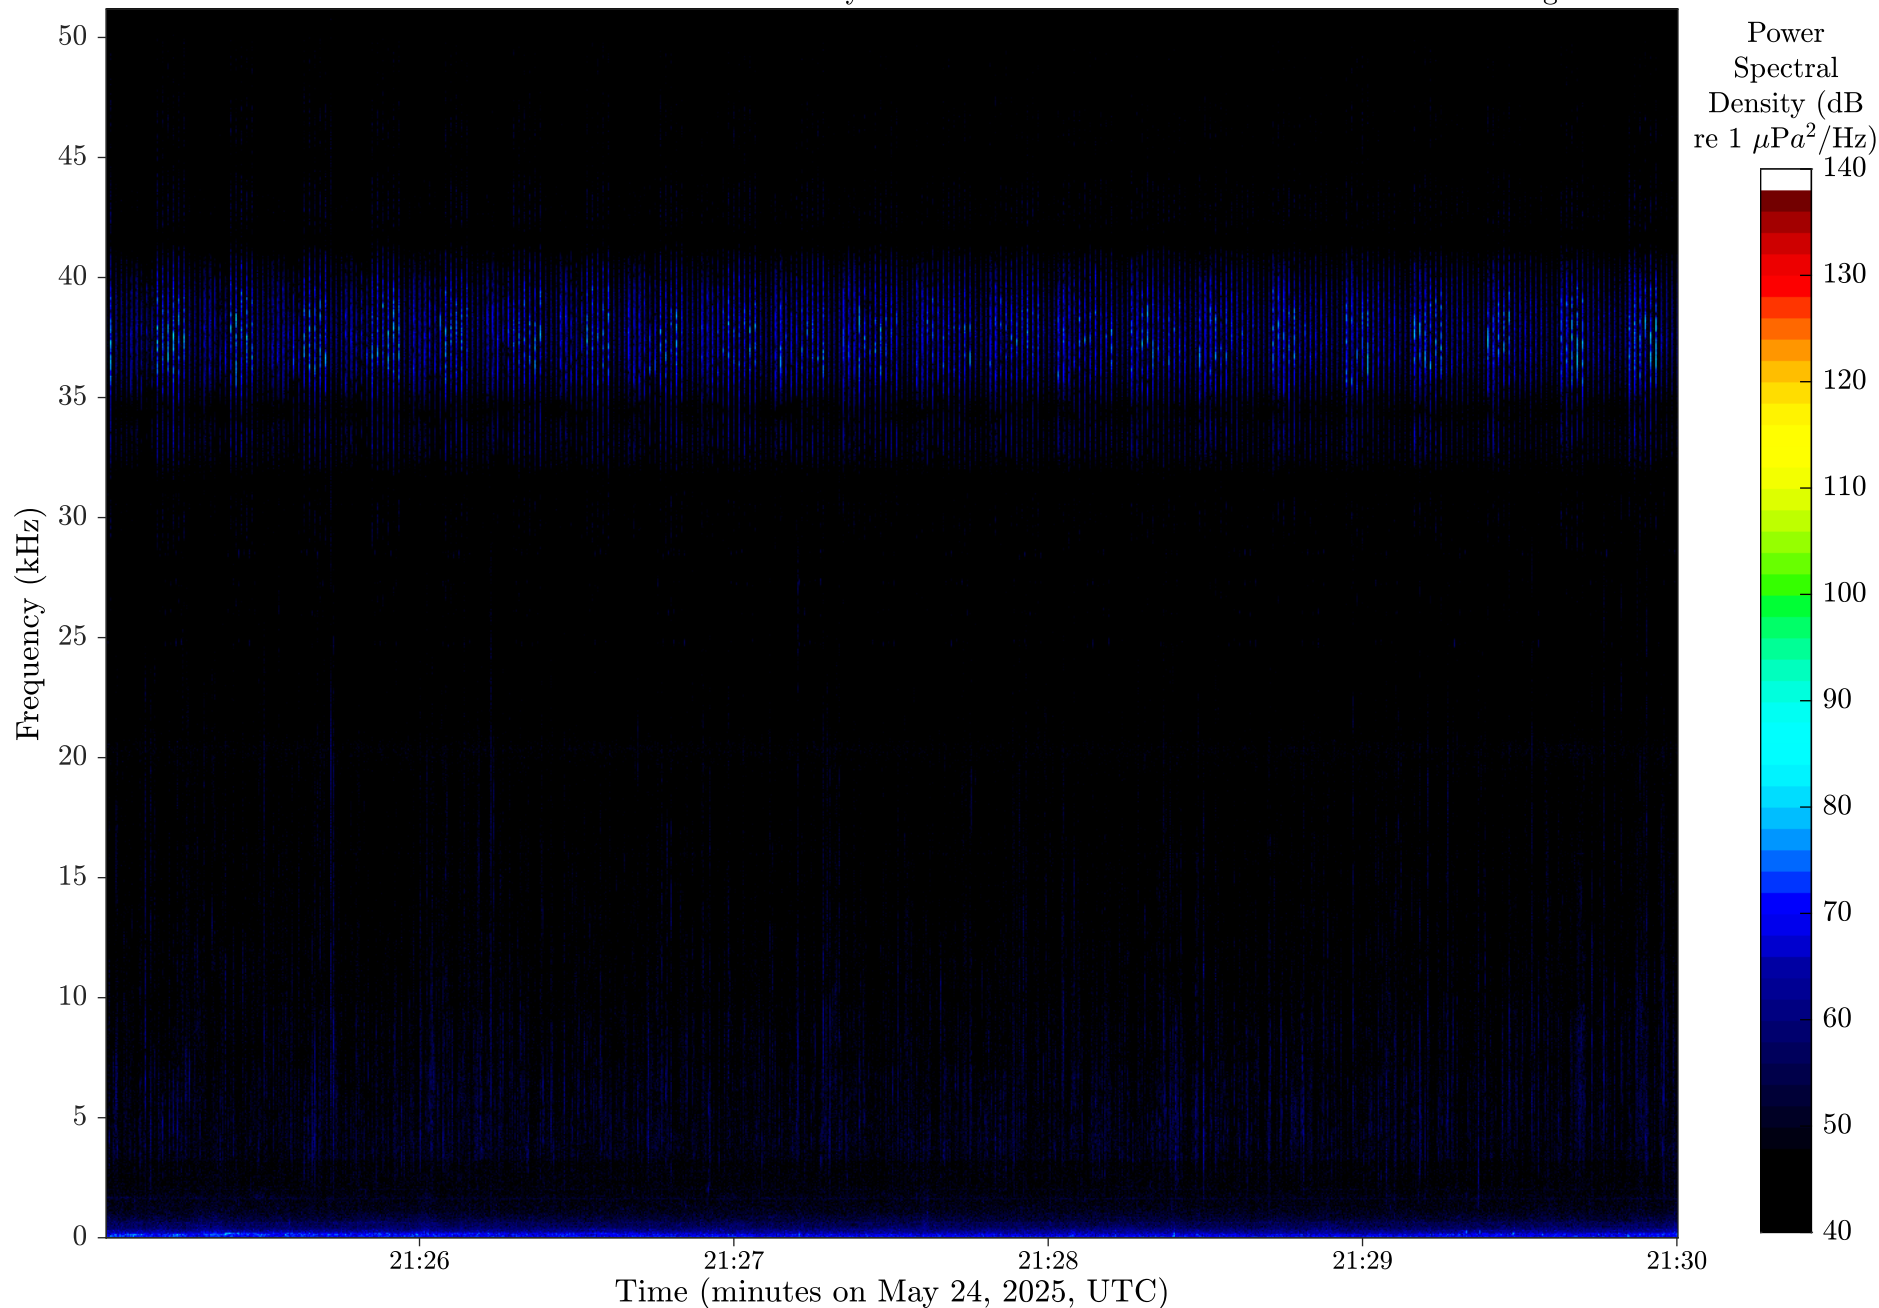


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:53:59 UTC

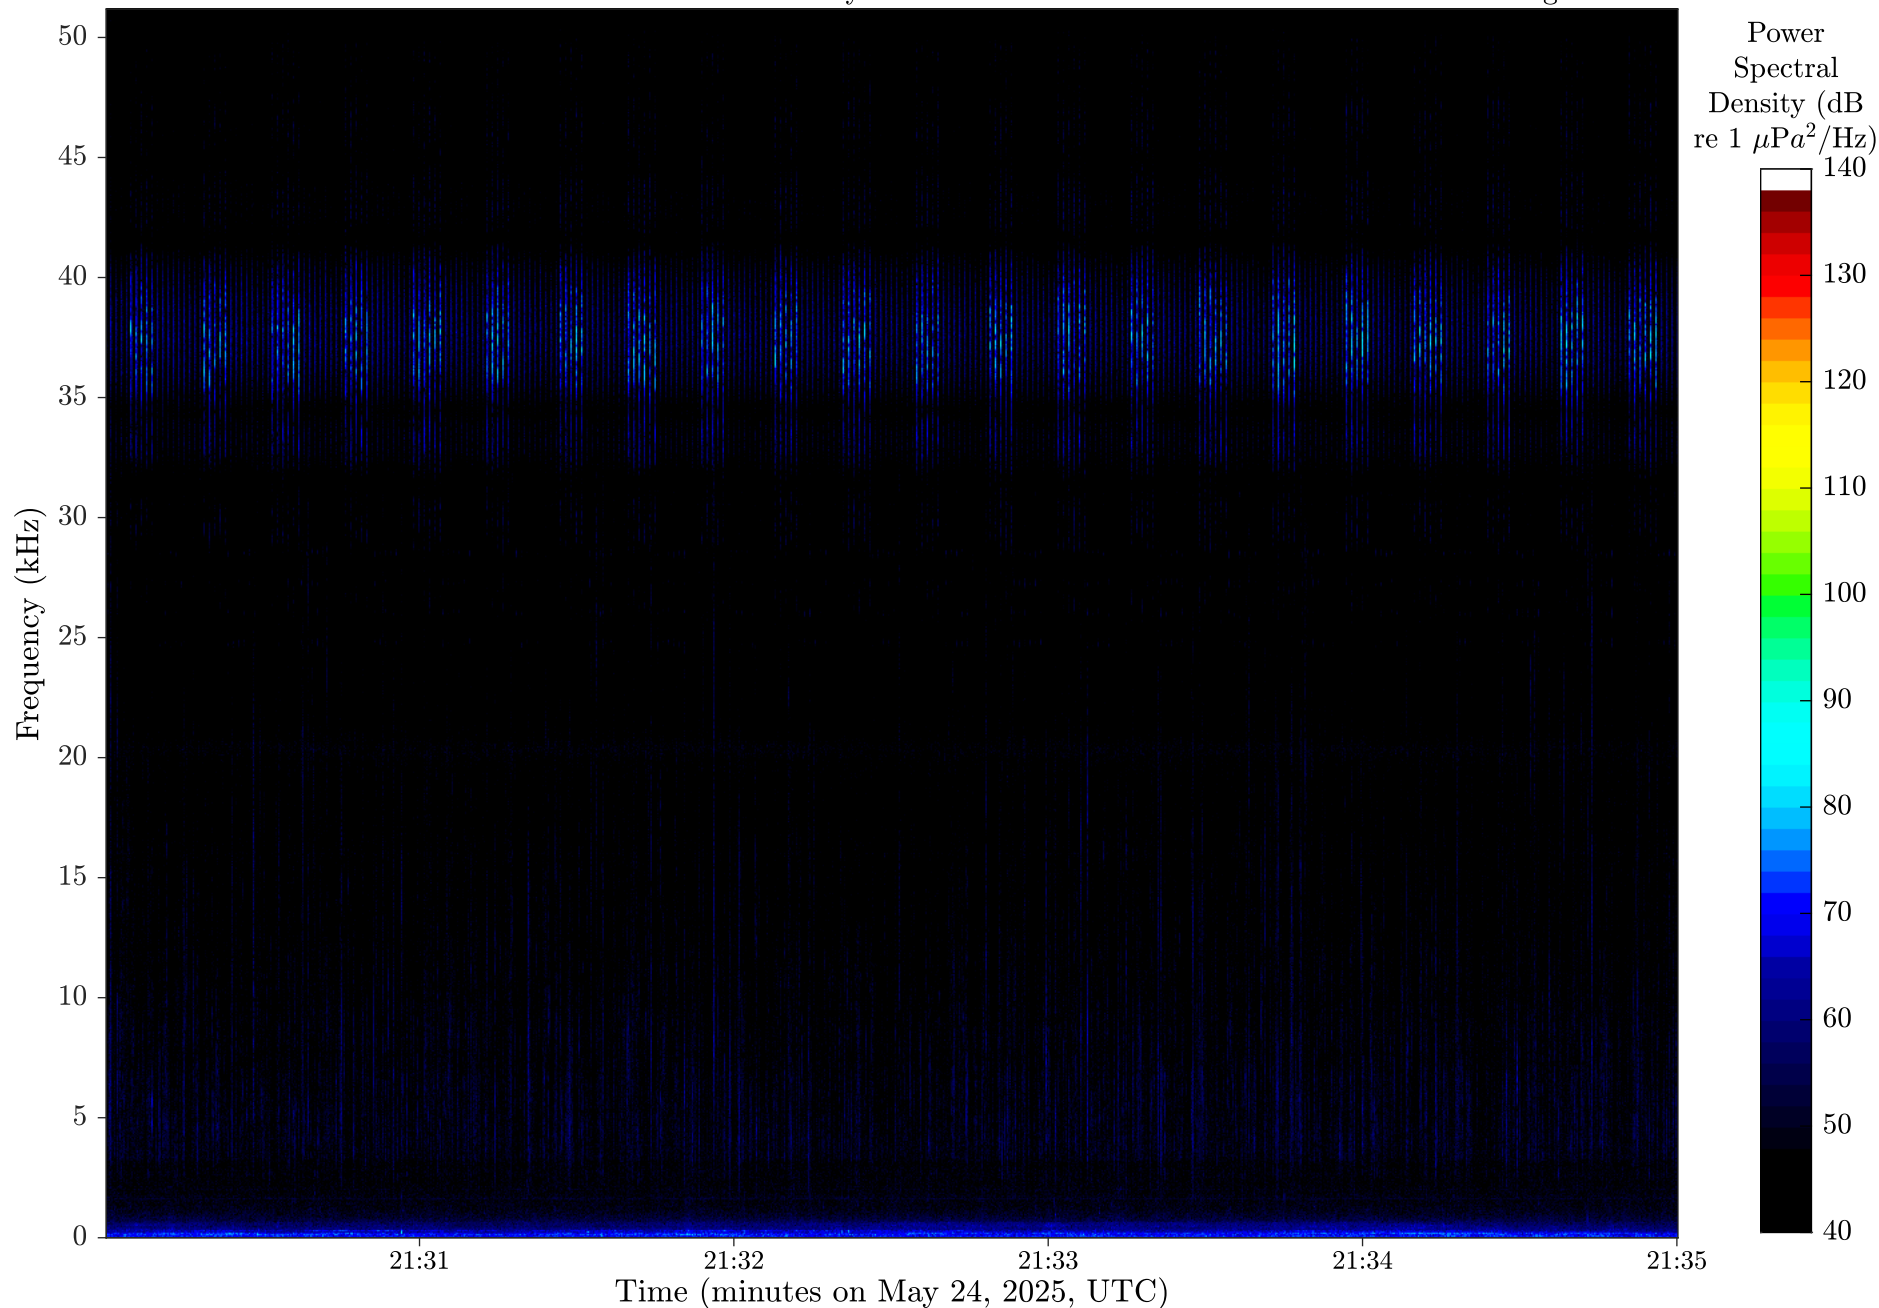


Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:54:07 UTC

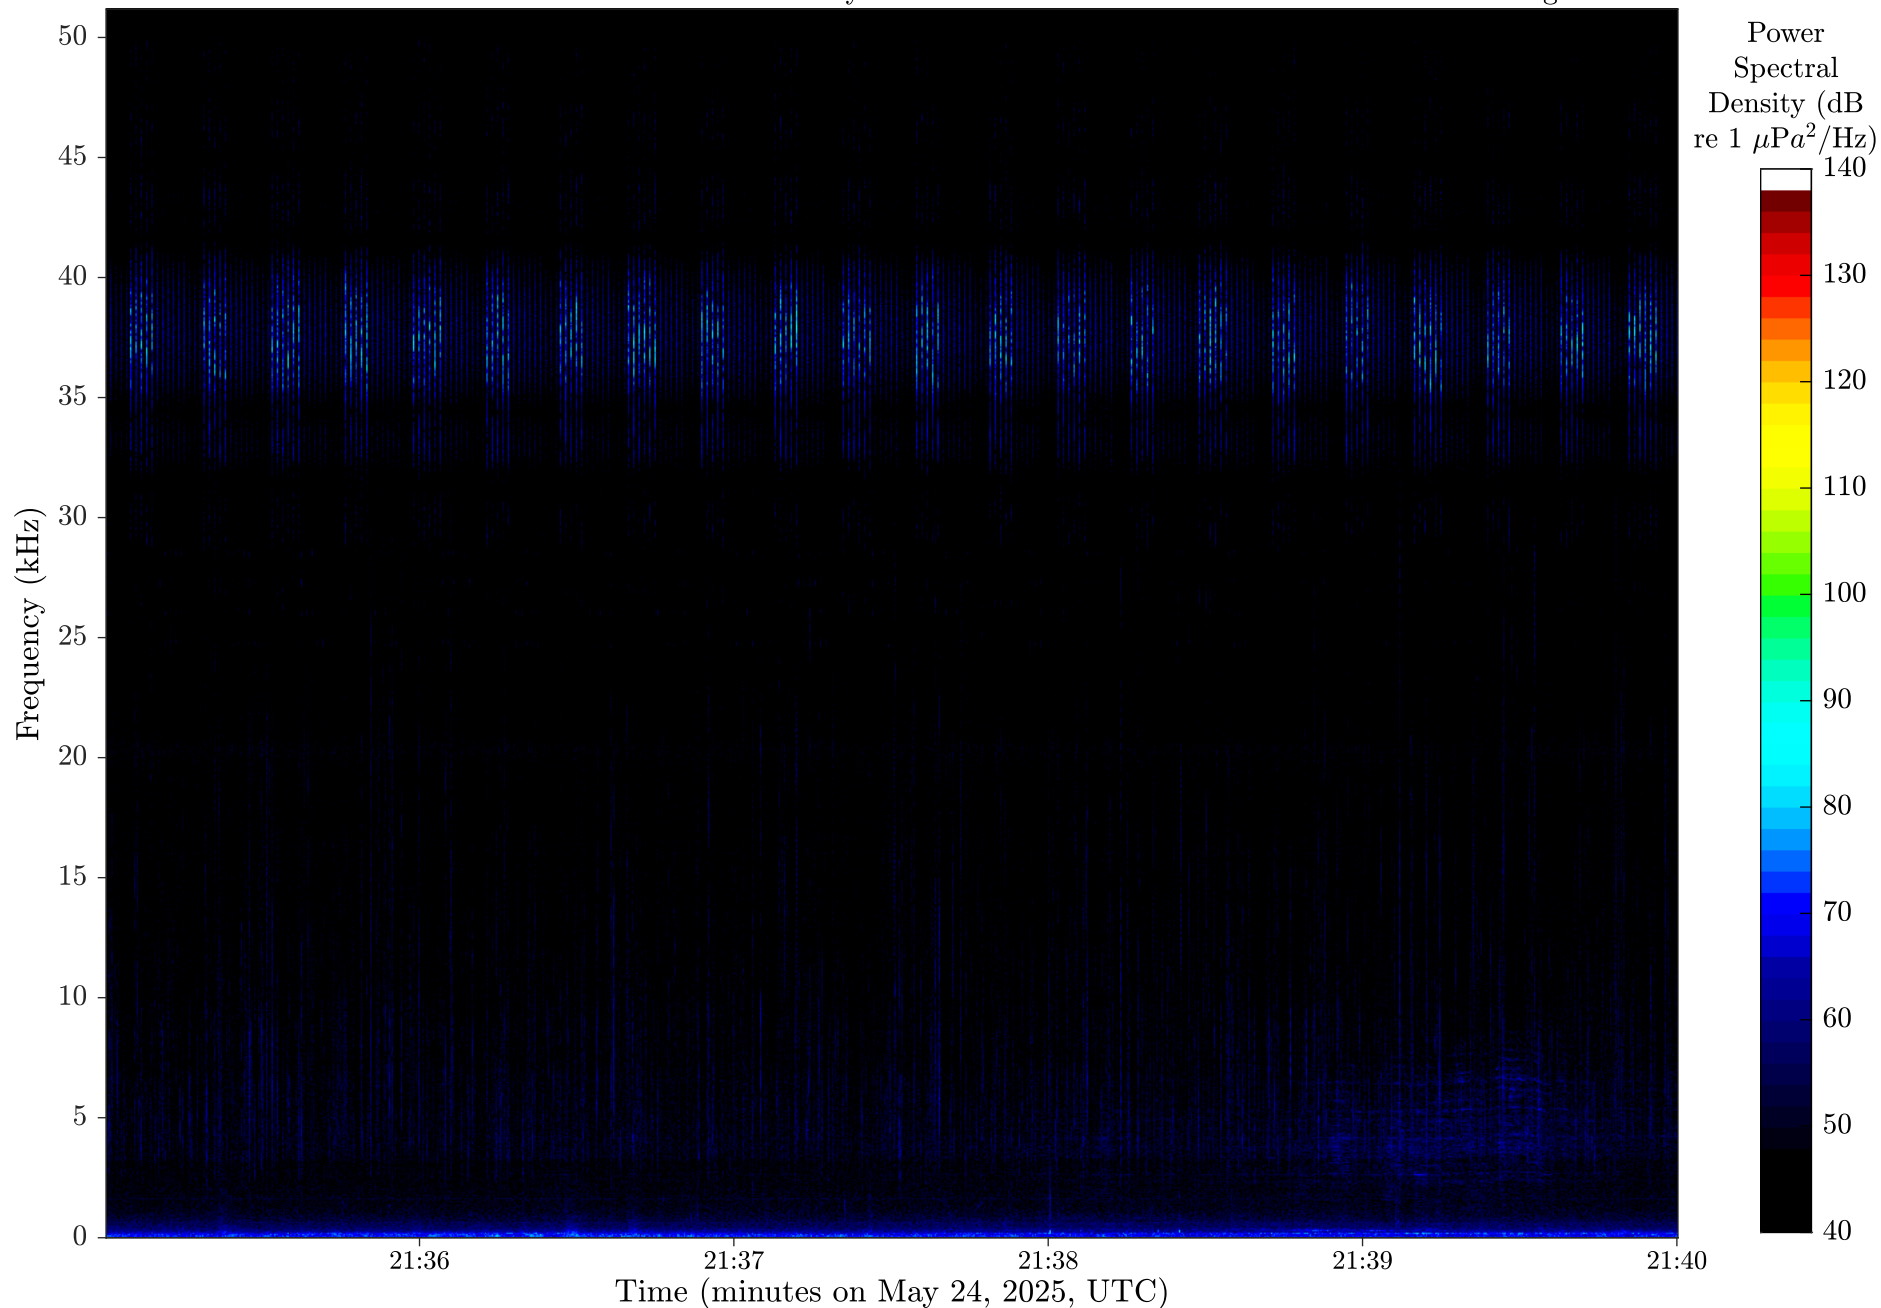


Comments: 33.8 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:54:15 UTC

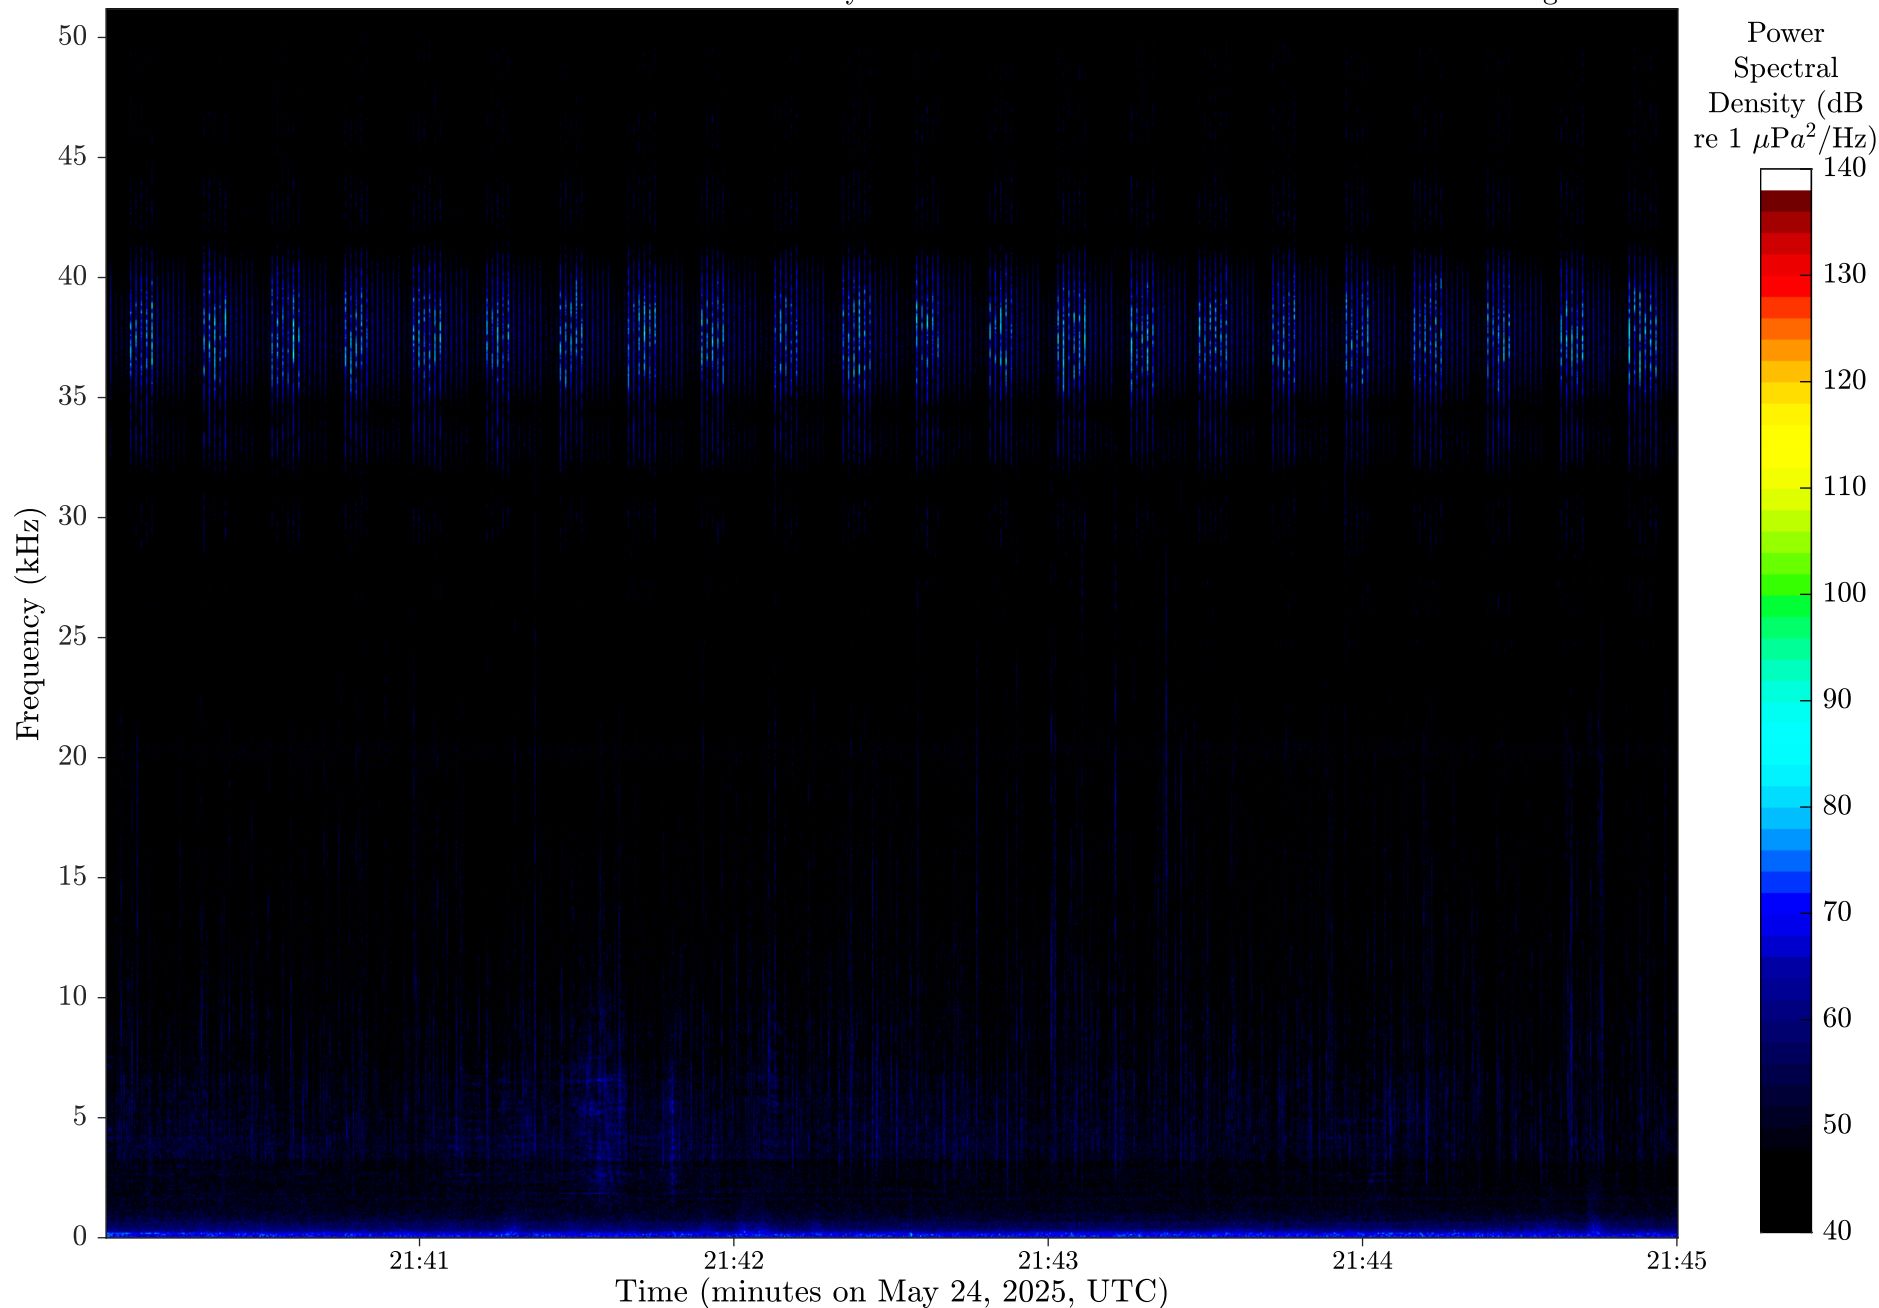

Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:54:22 UTC

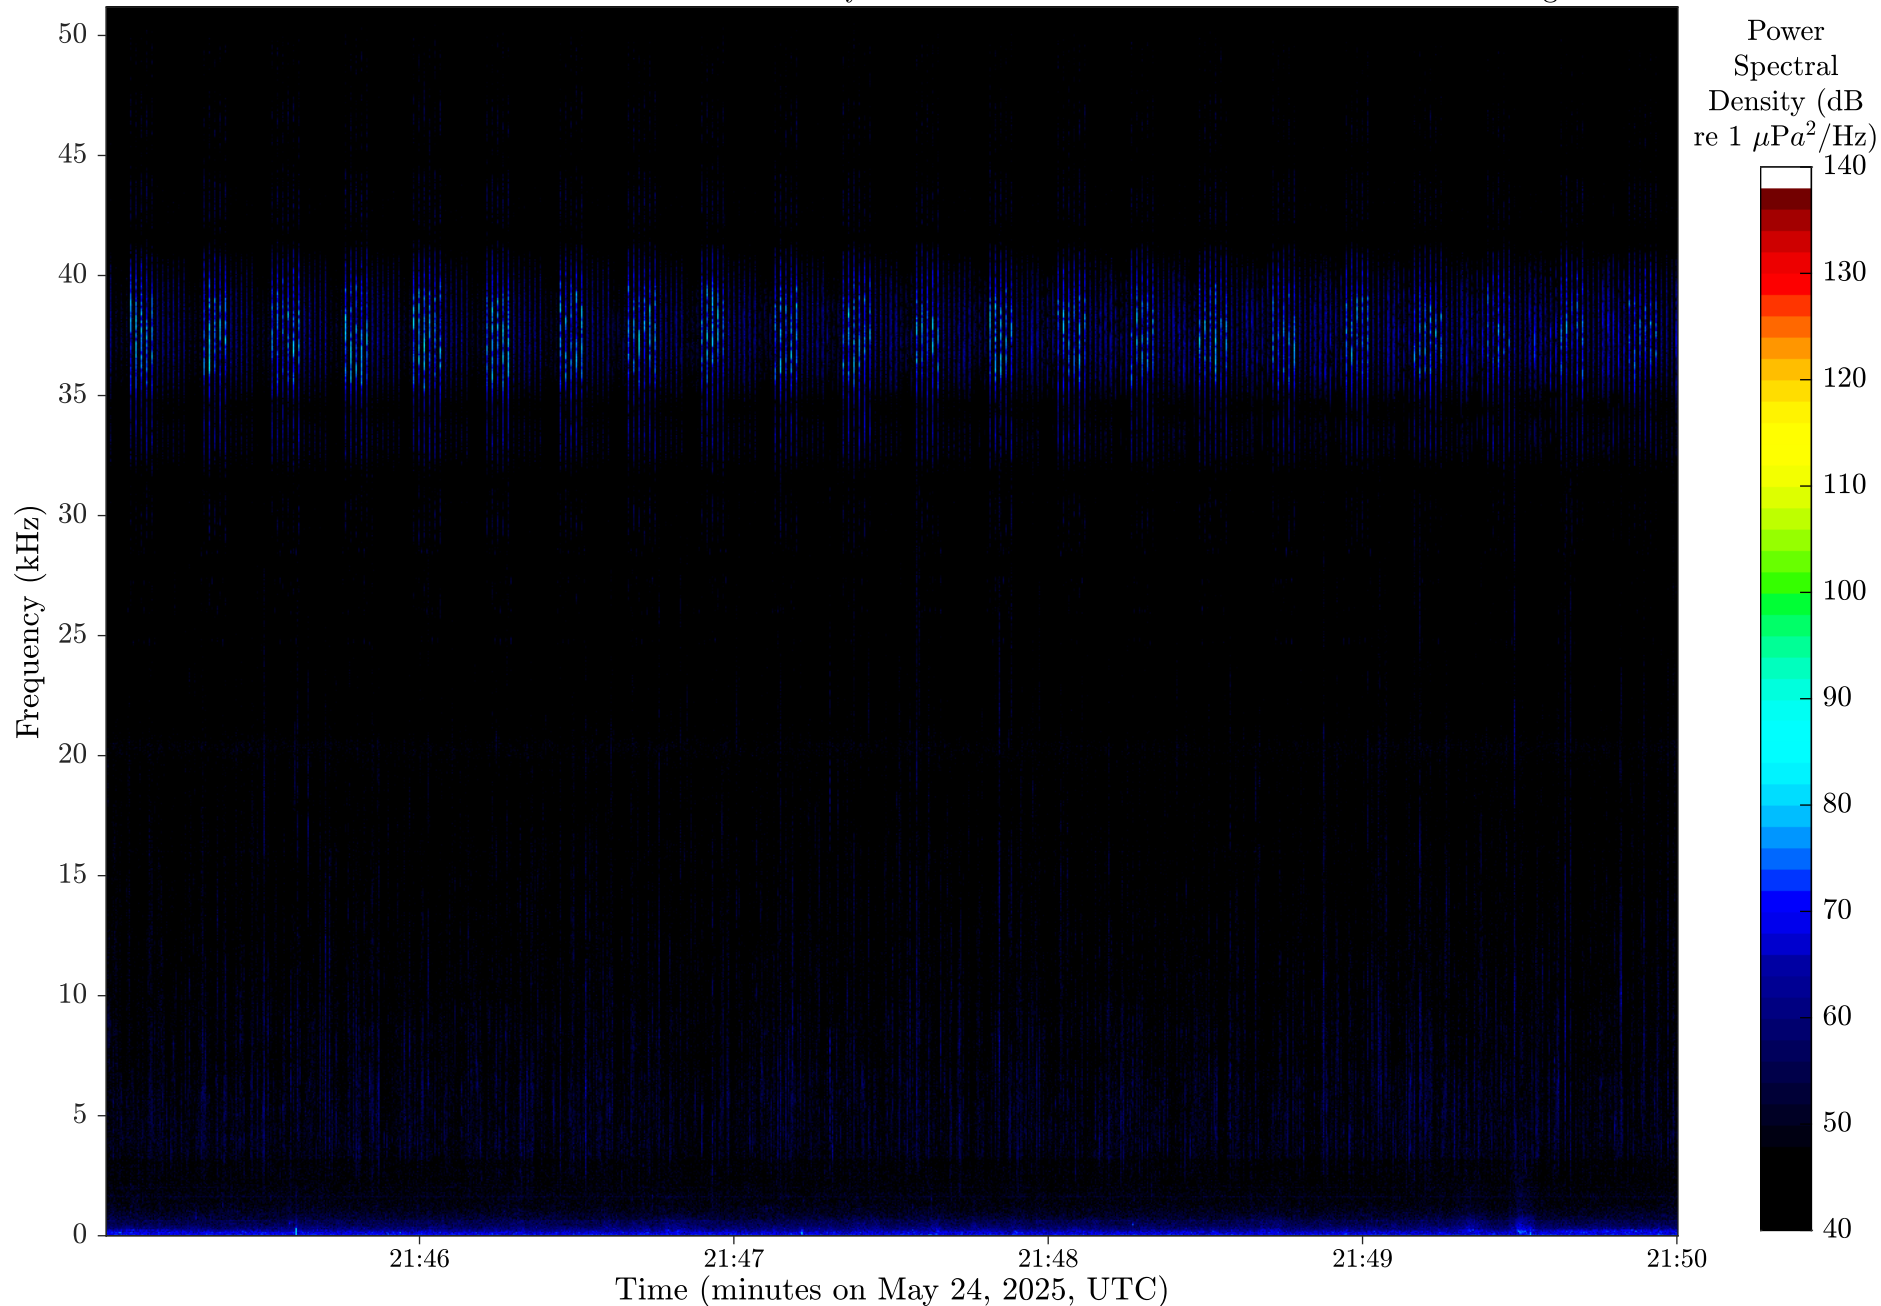

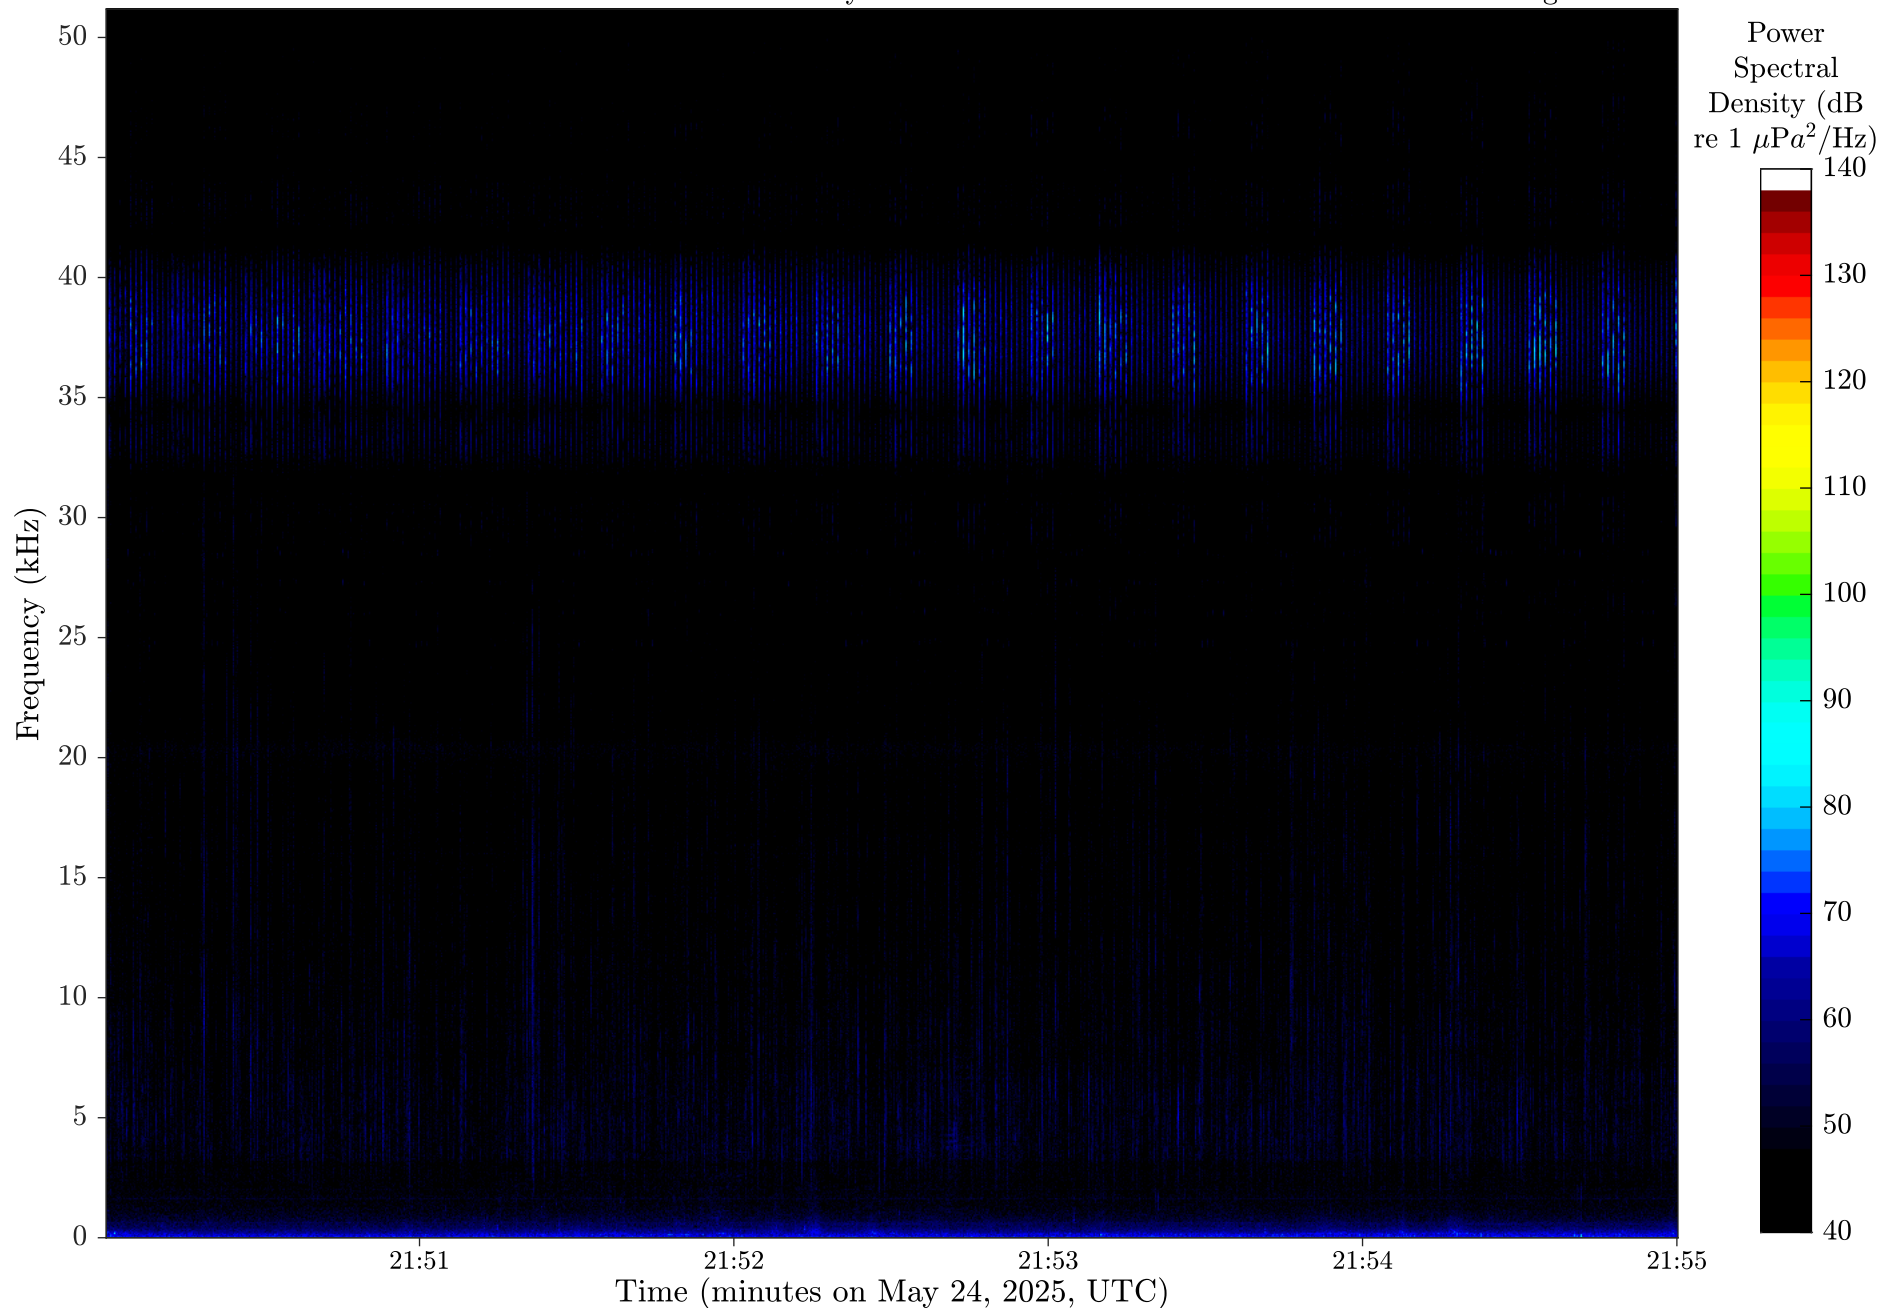


Comments: 33.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:54:38 UTC

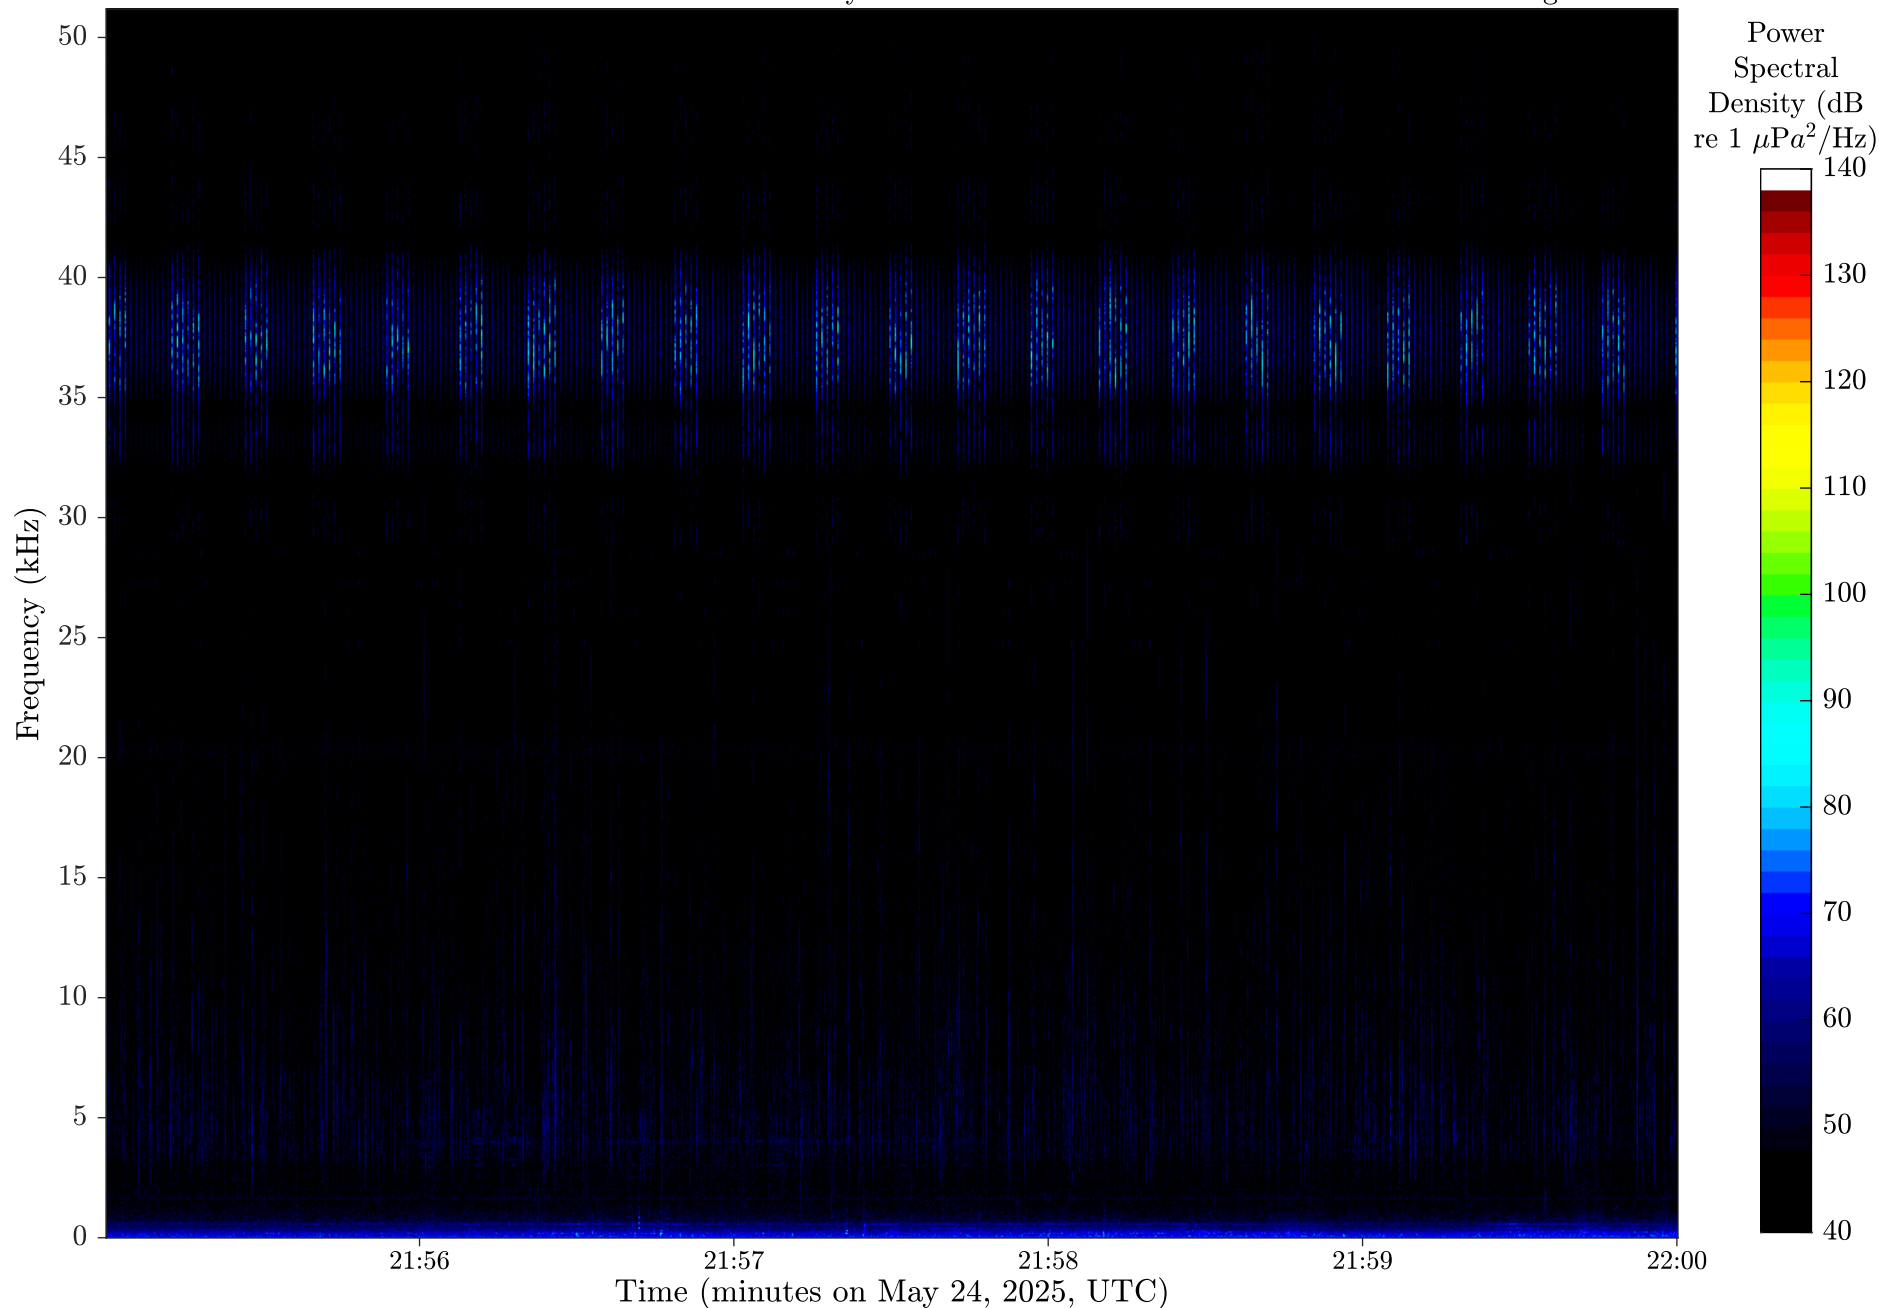


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:54:45 UTC

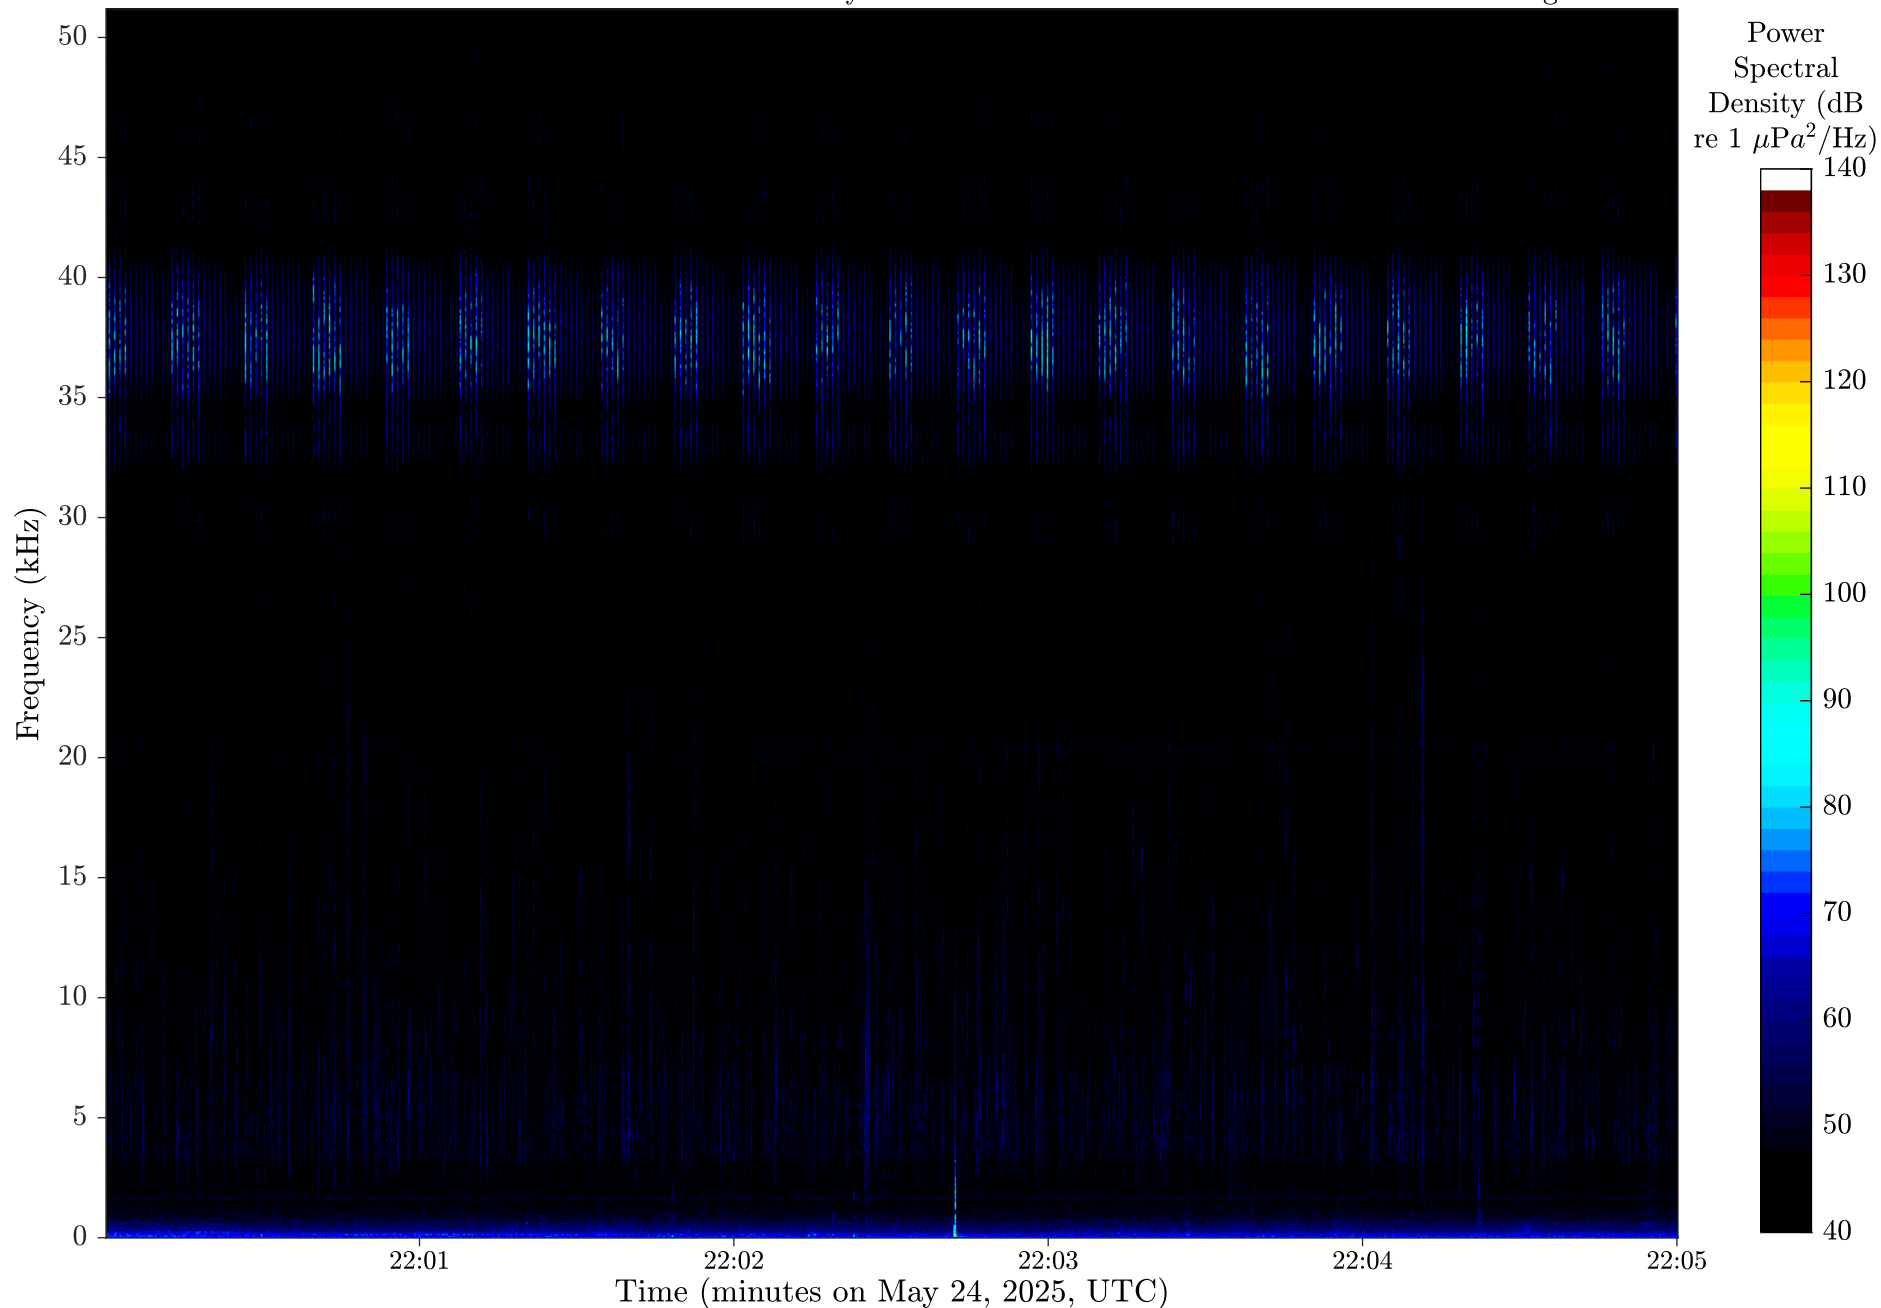

Comments: 35.1 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:54:52 UTC

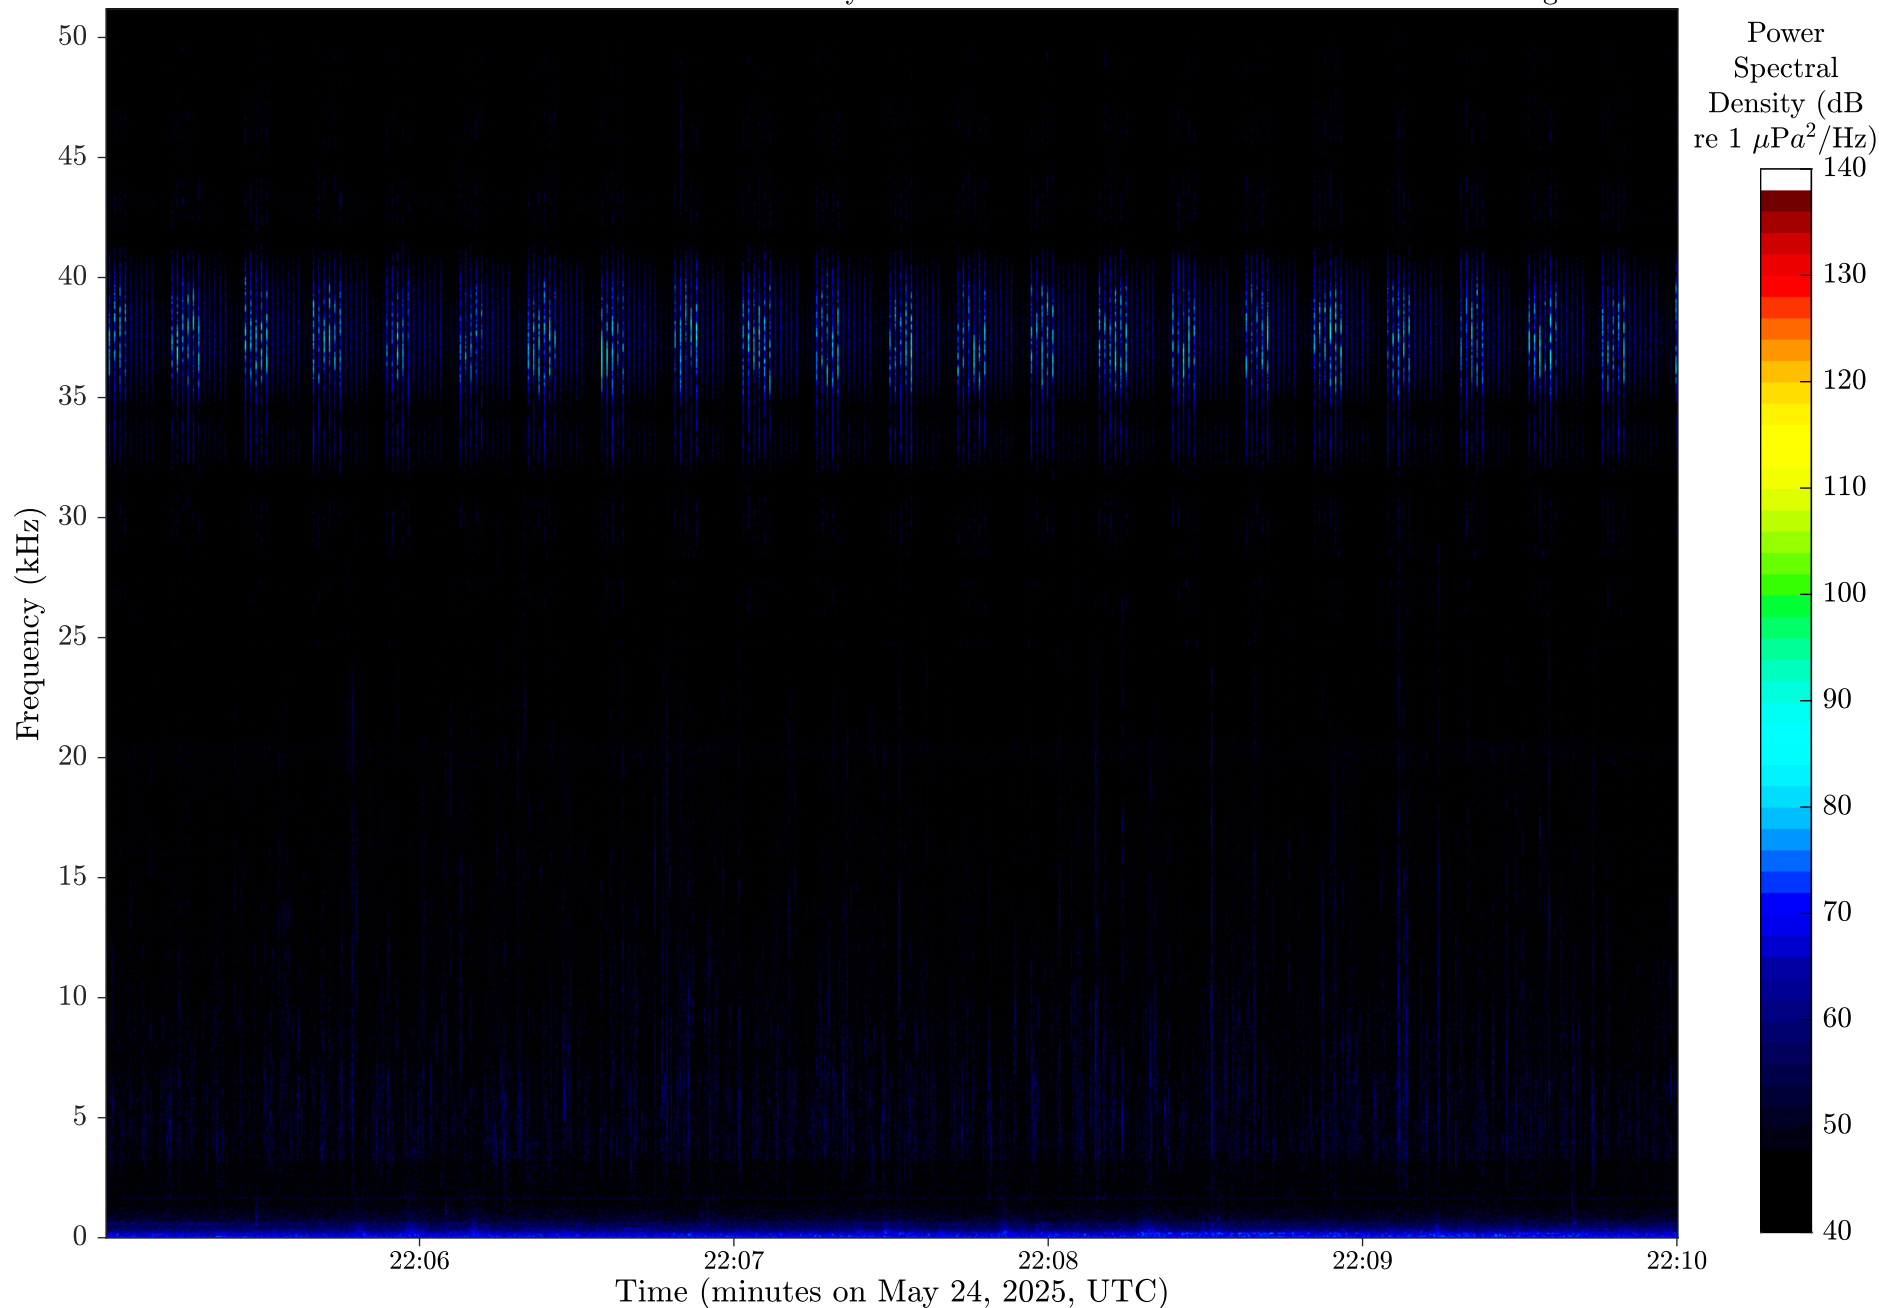

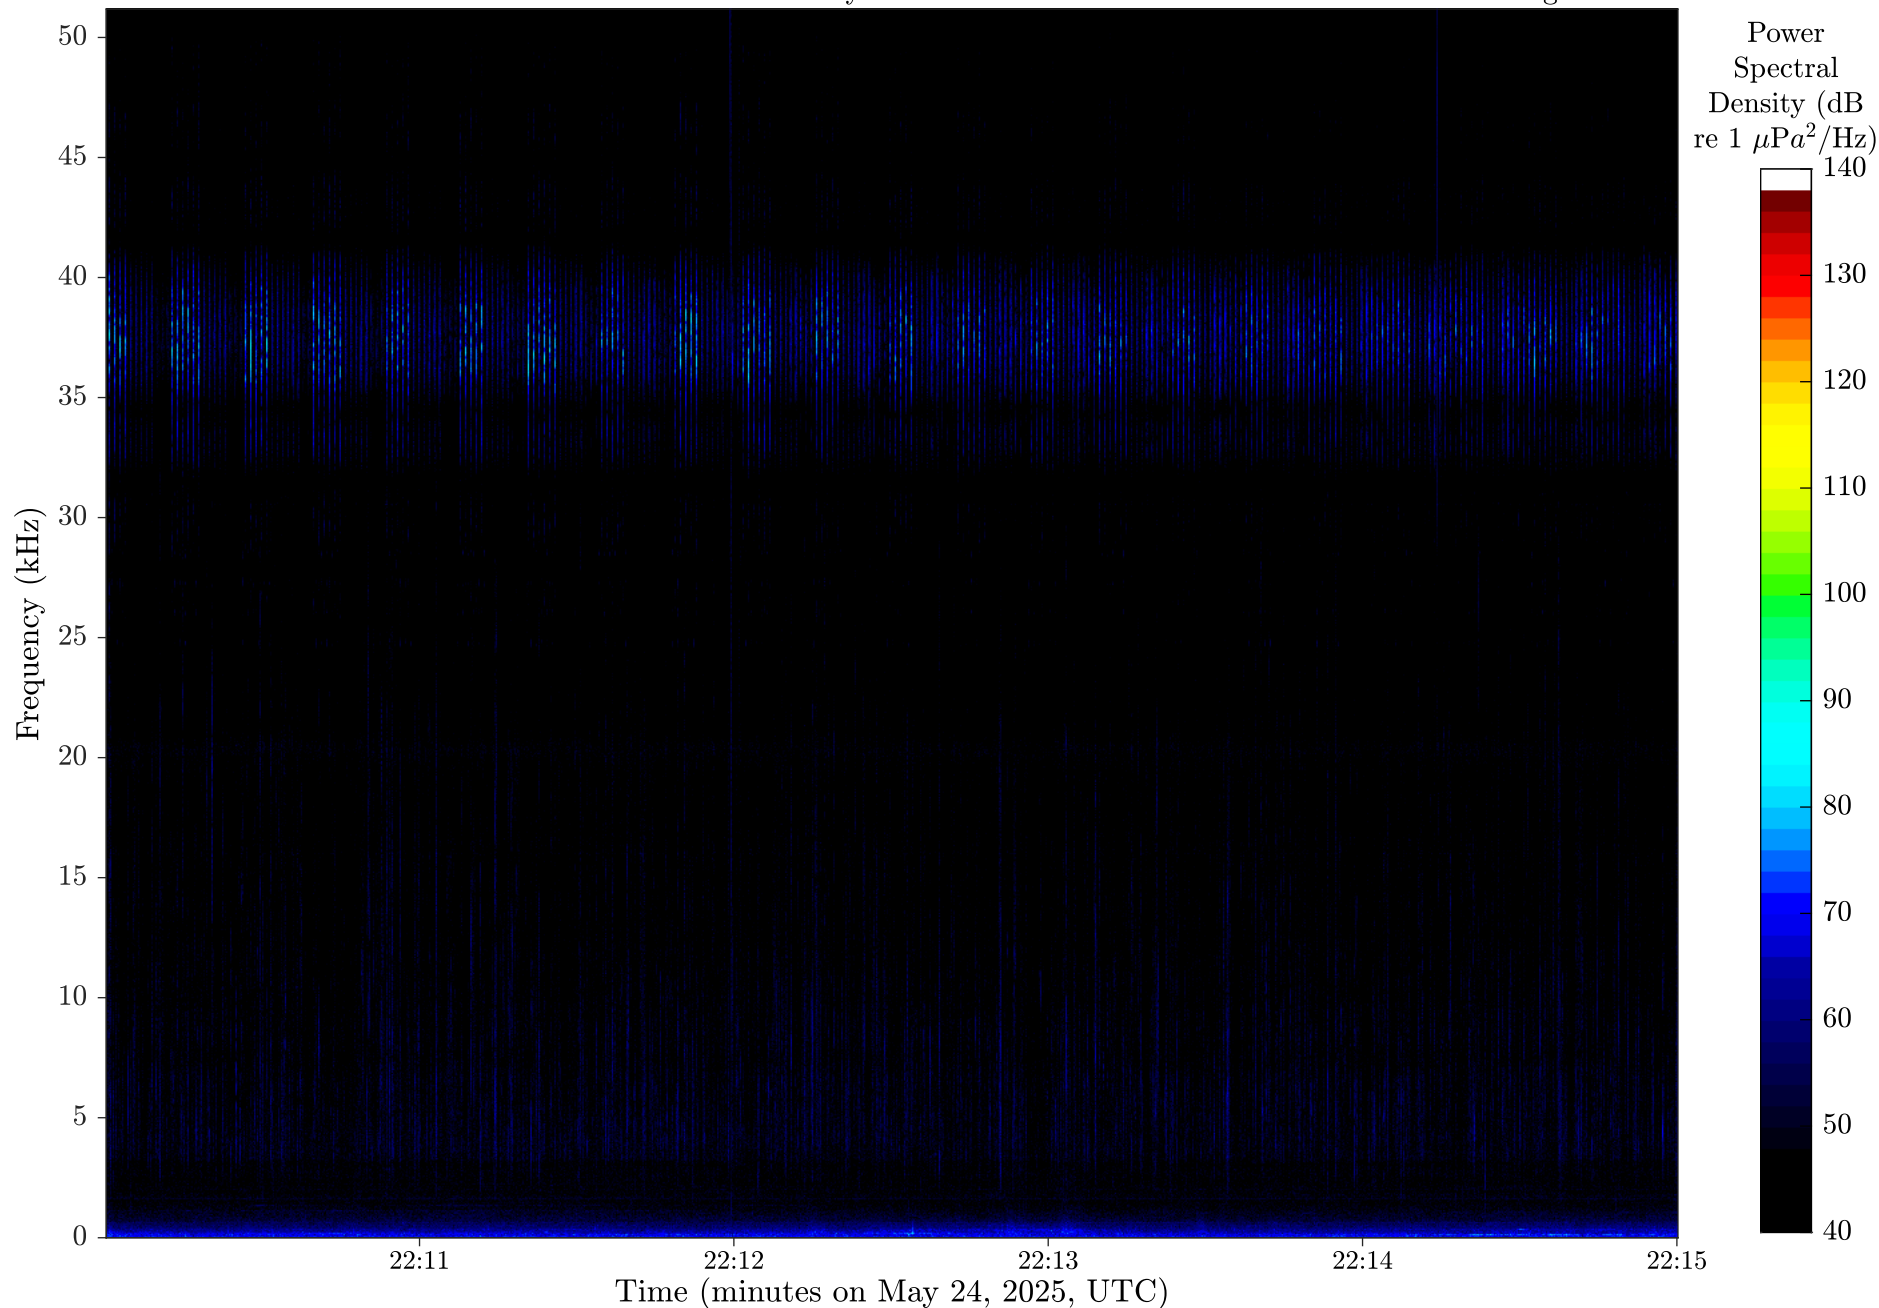


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:55:08 UTC

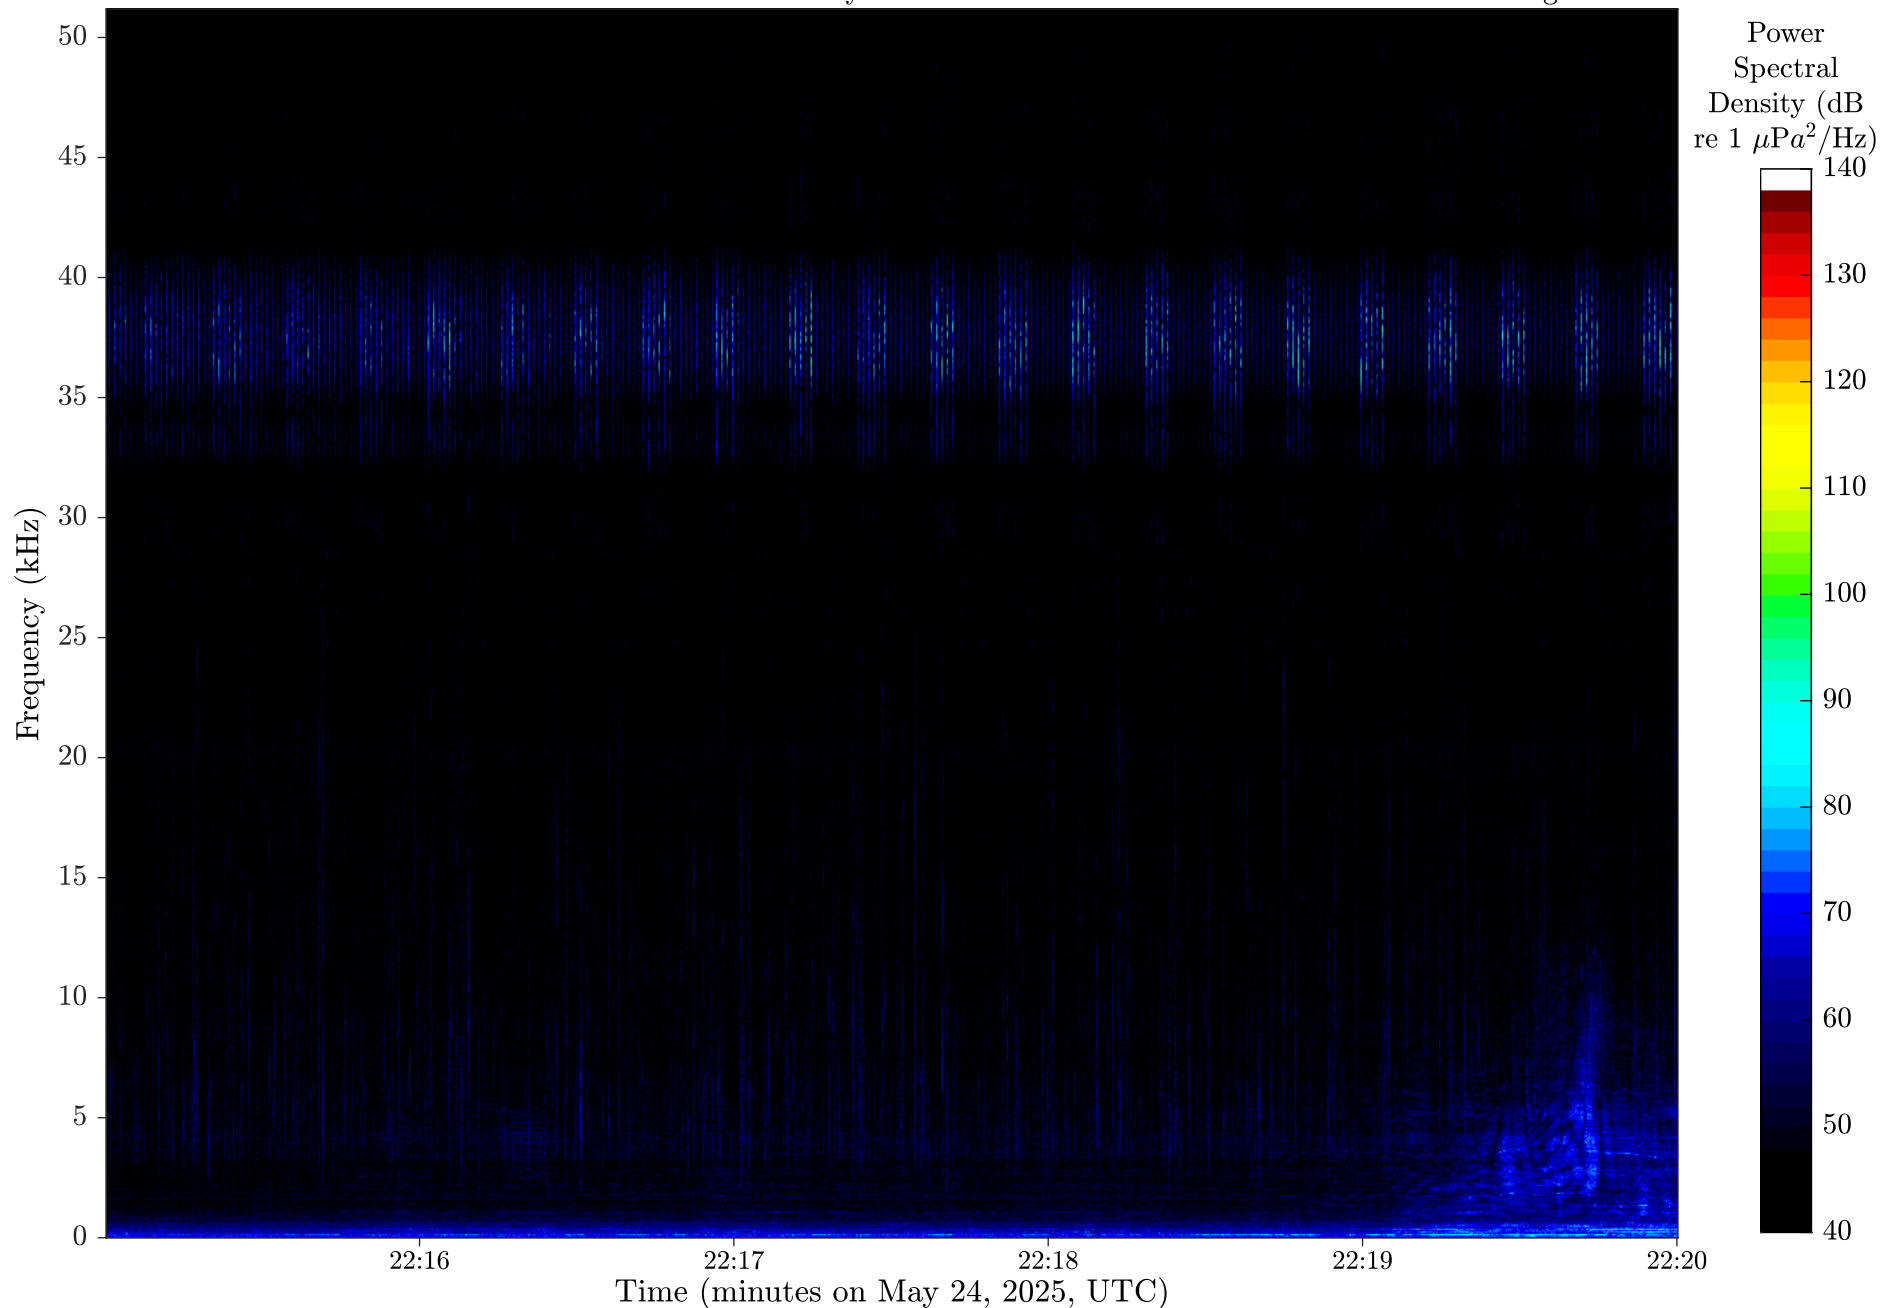

Comments: 33.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:55:14 UTC

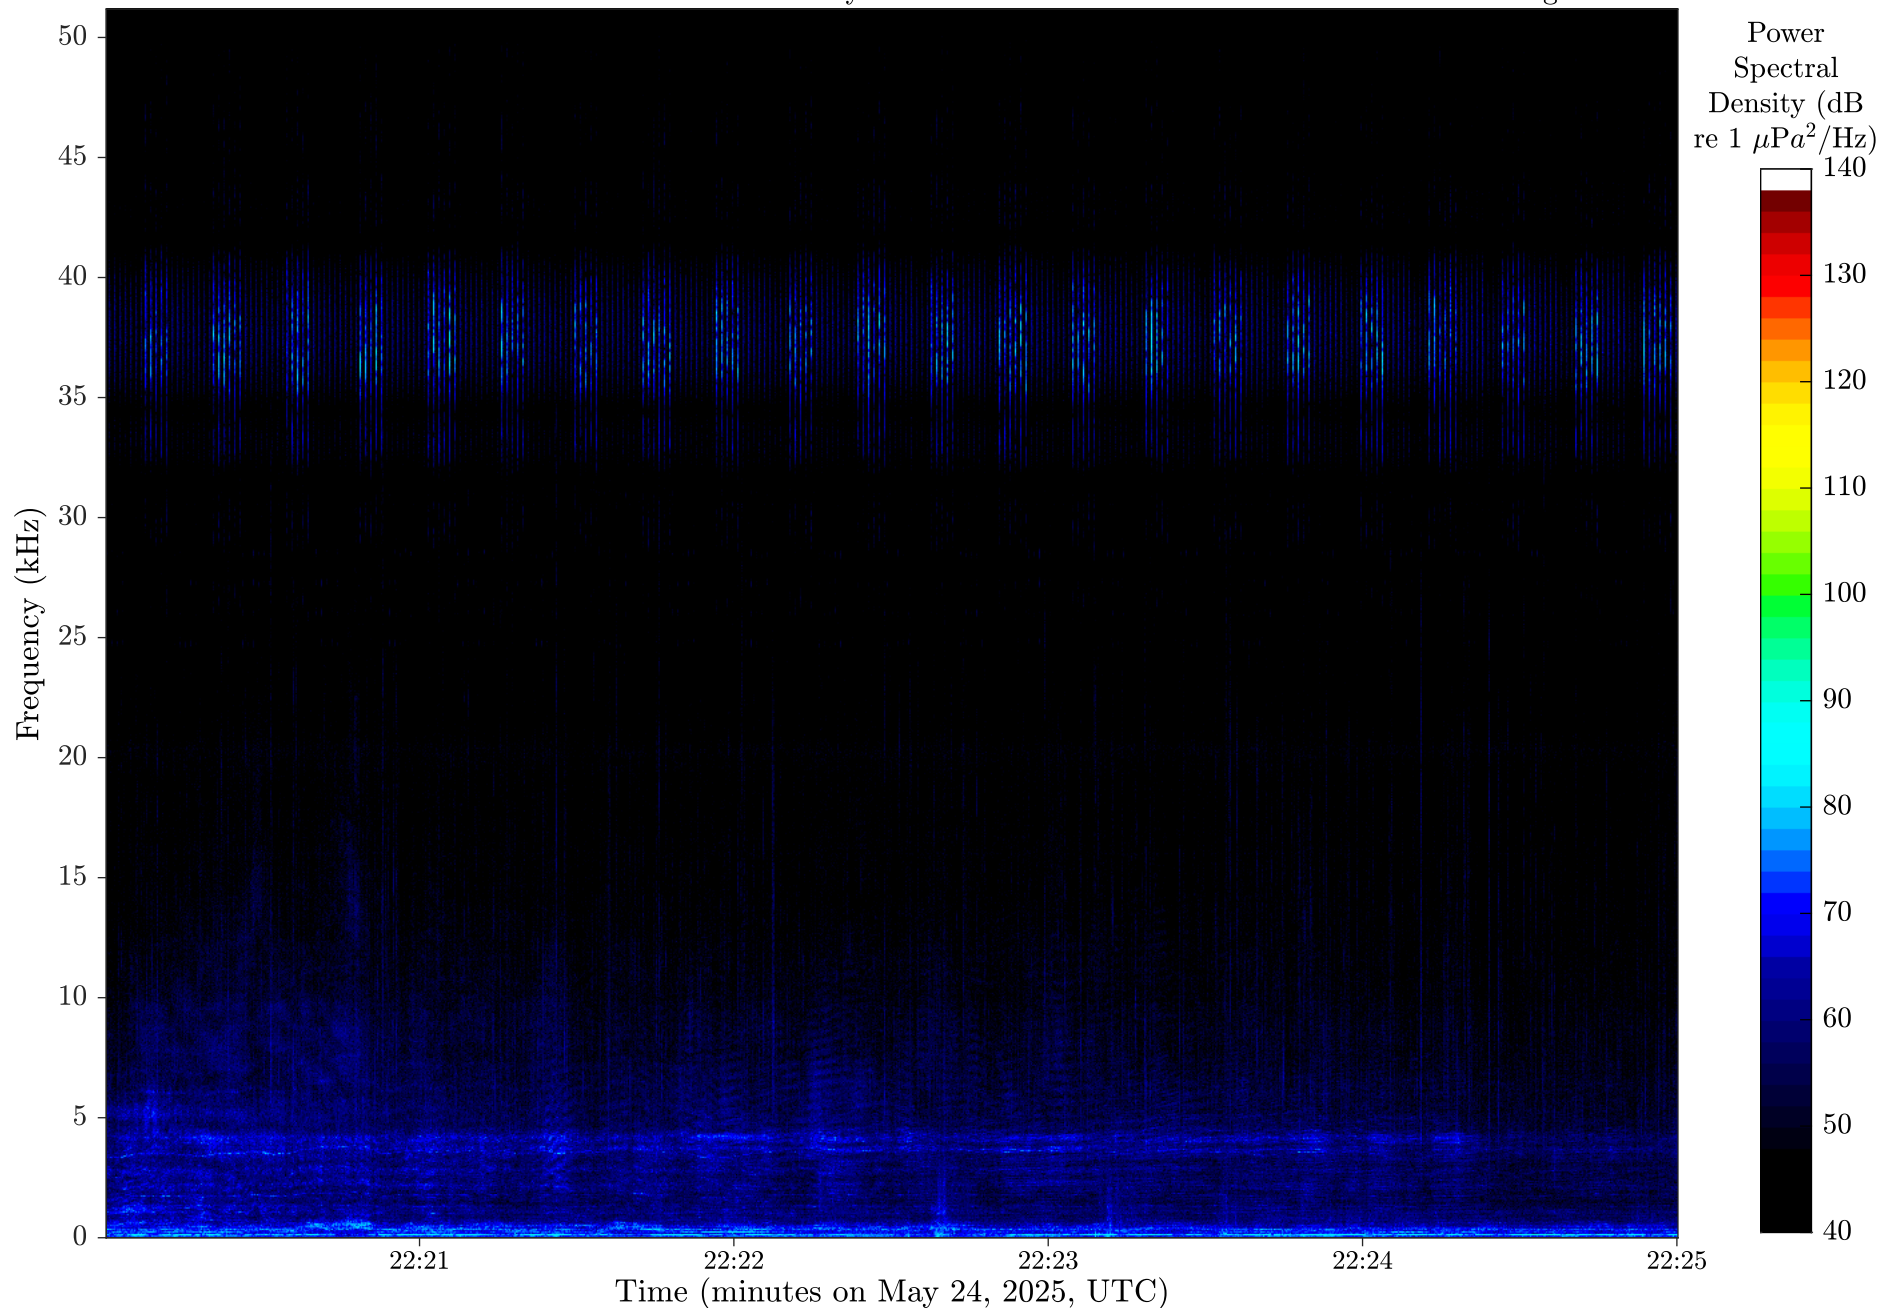

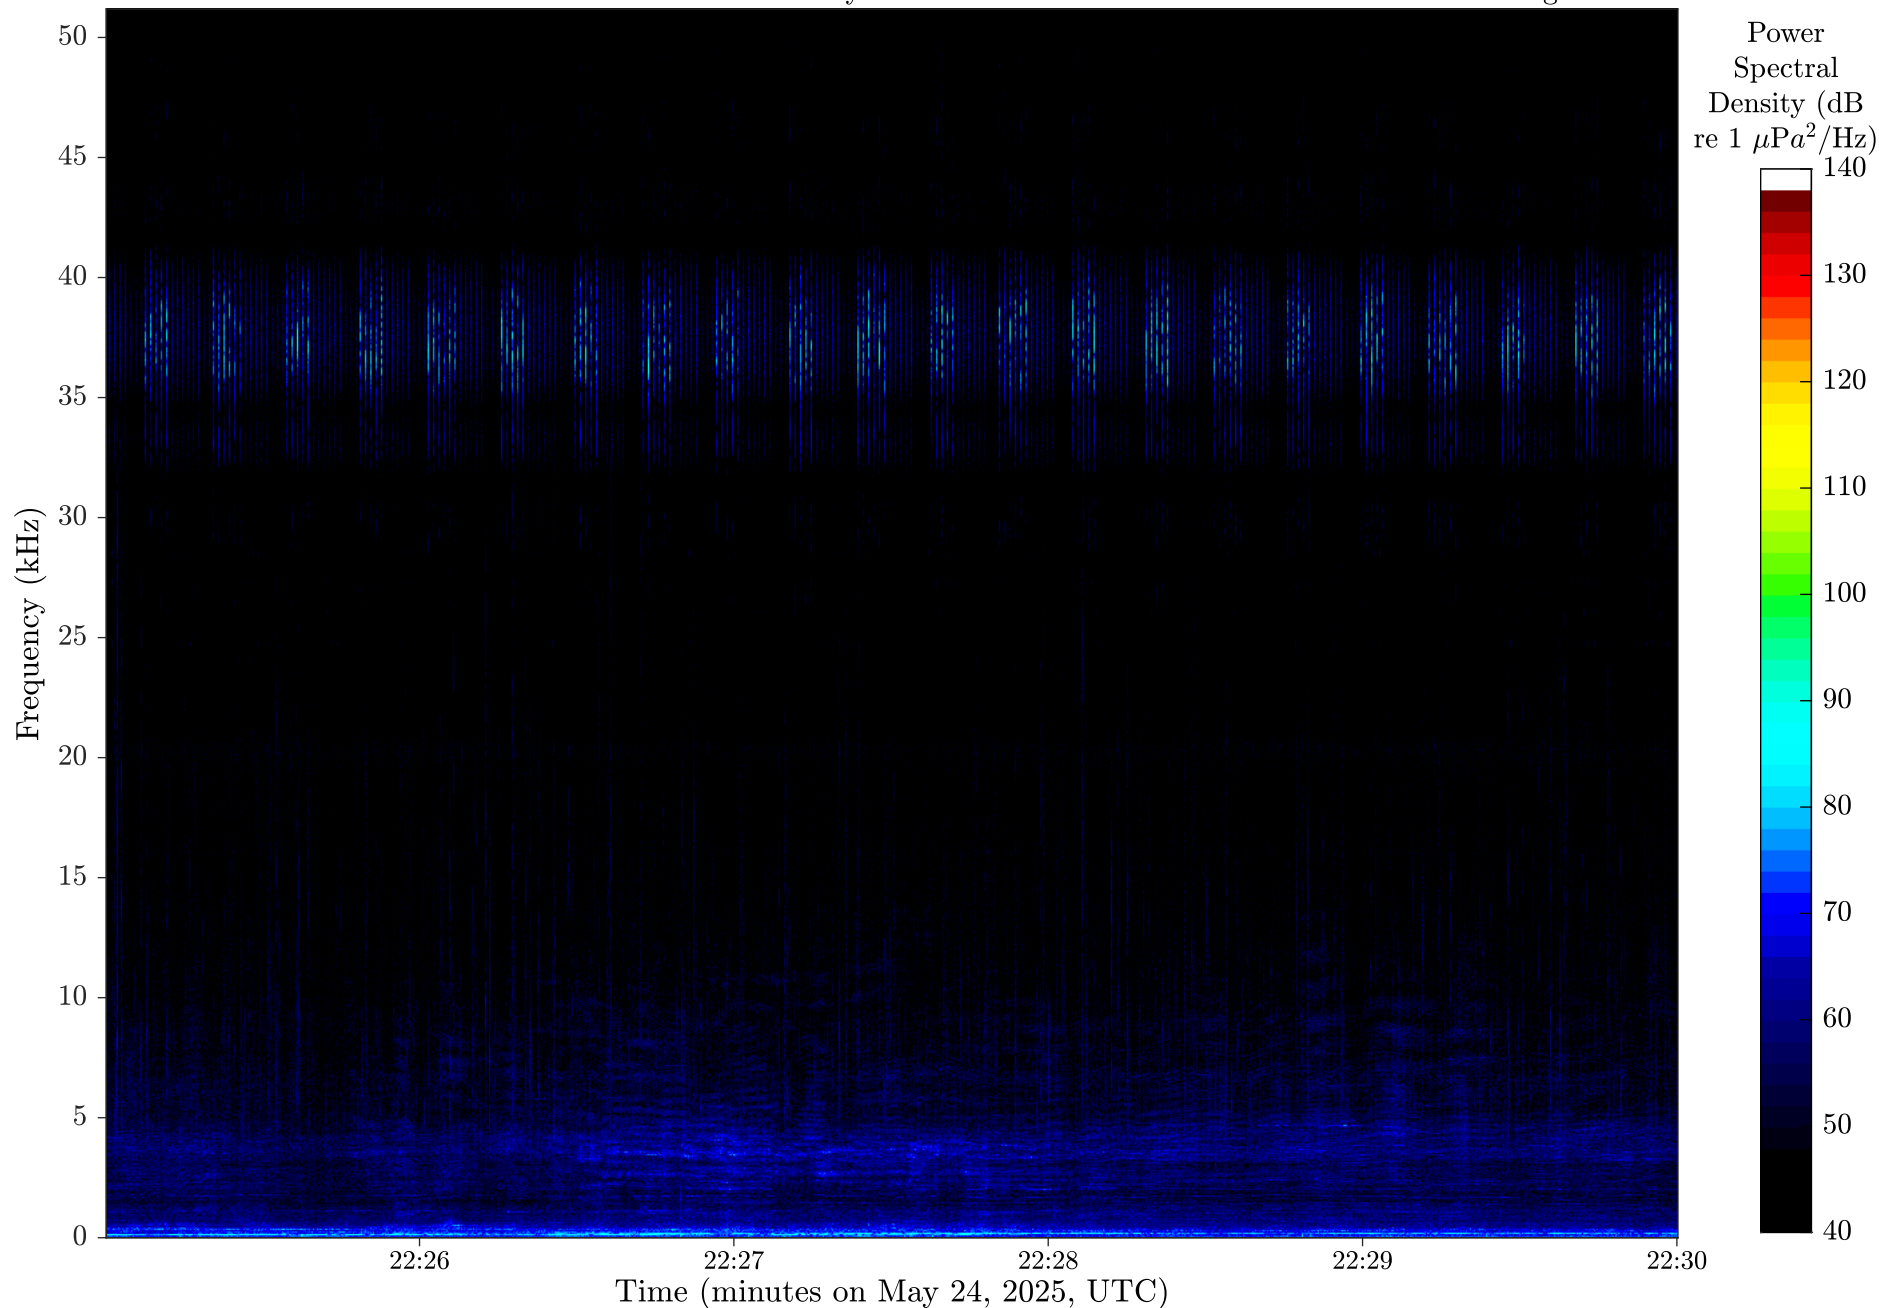


Comments: 34.2 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:55:29 UTC

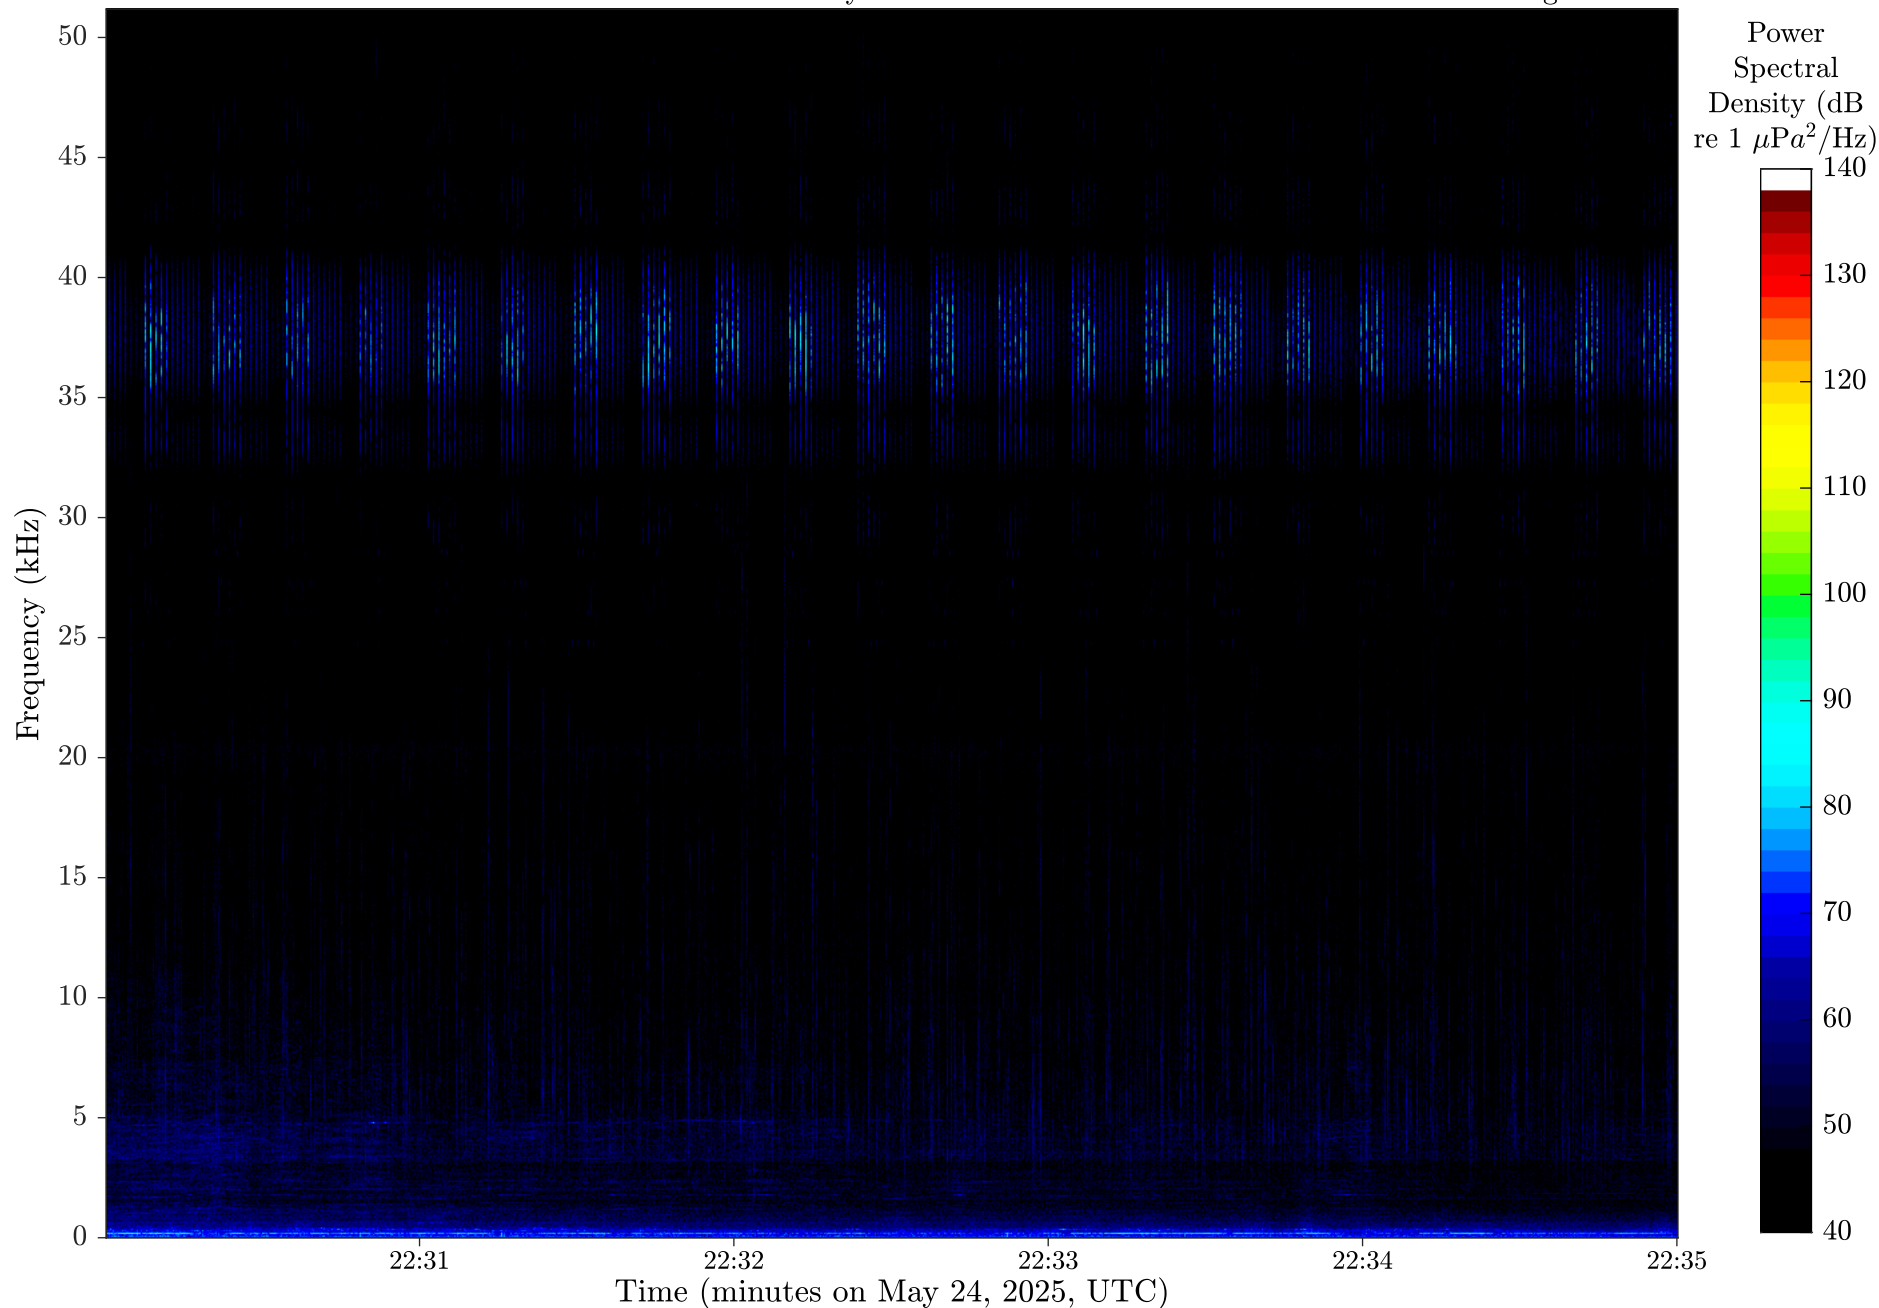

Comments: 34.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:55:36 UTC

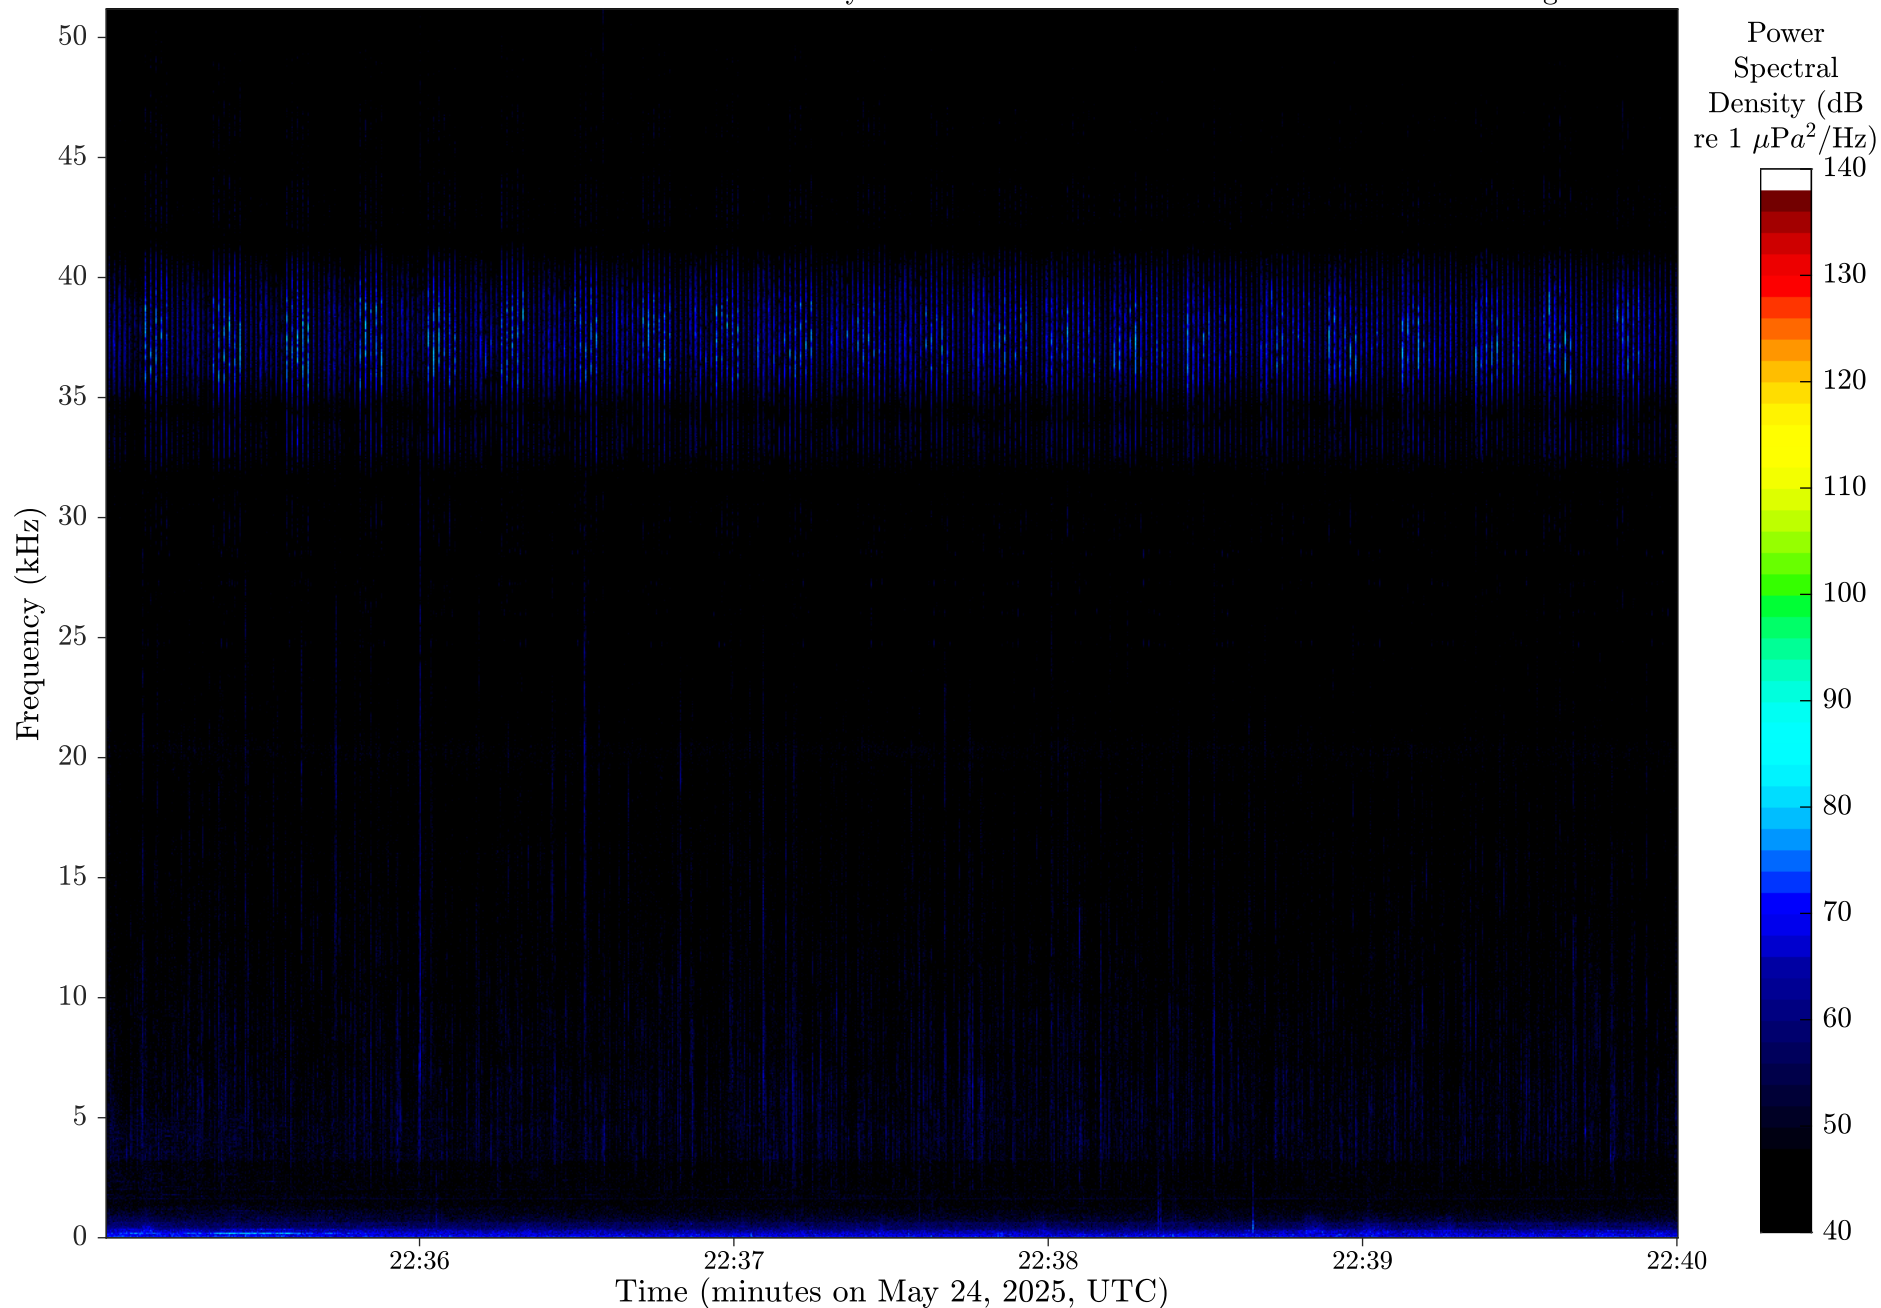

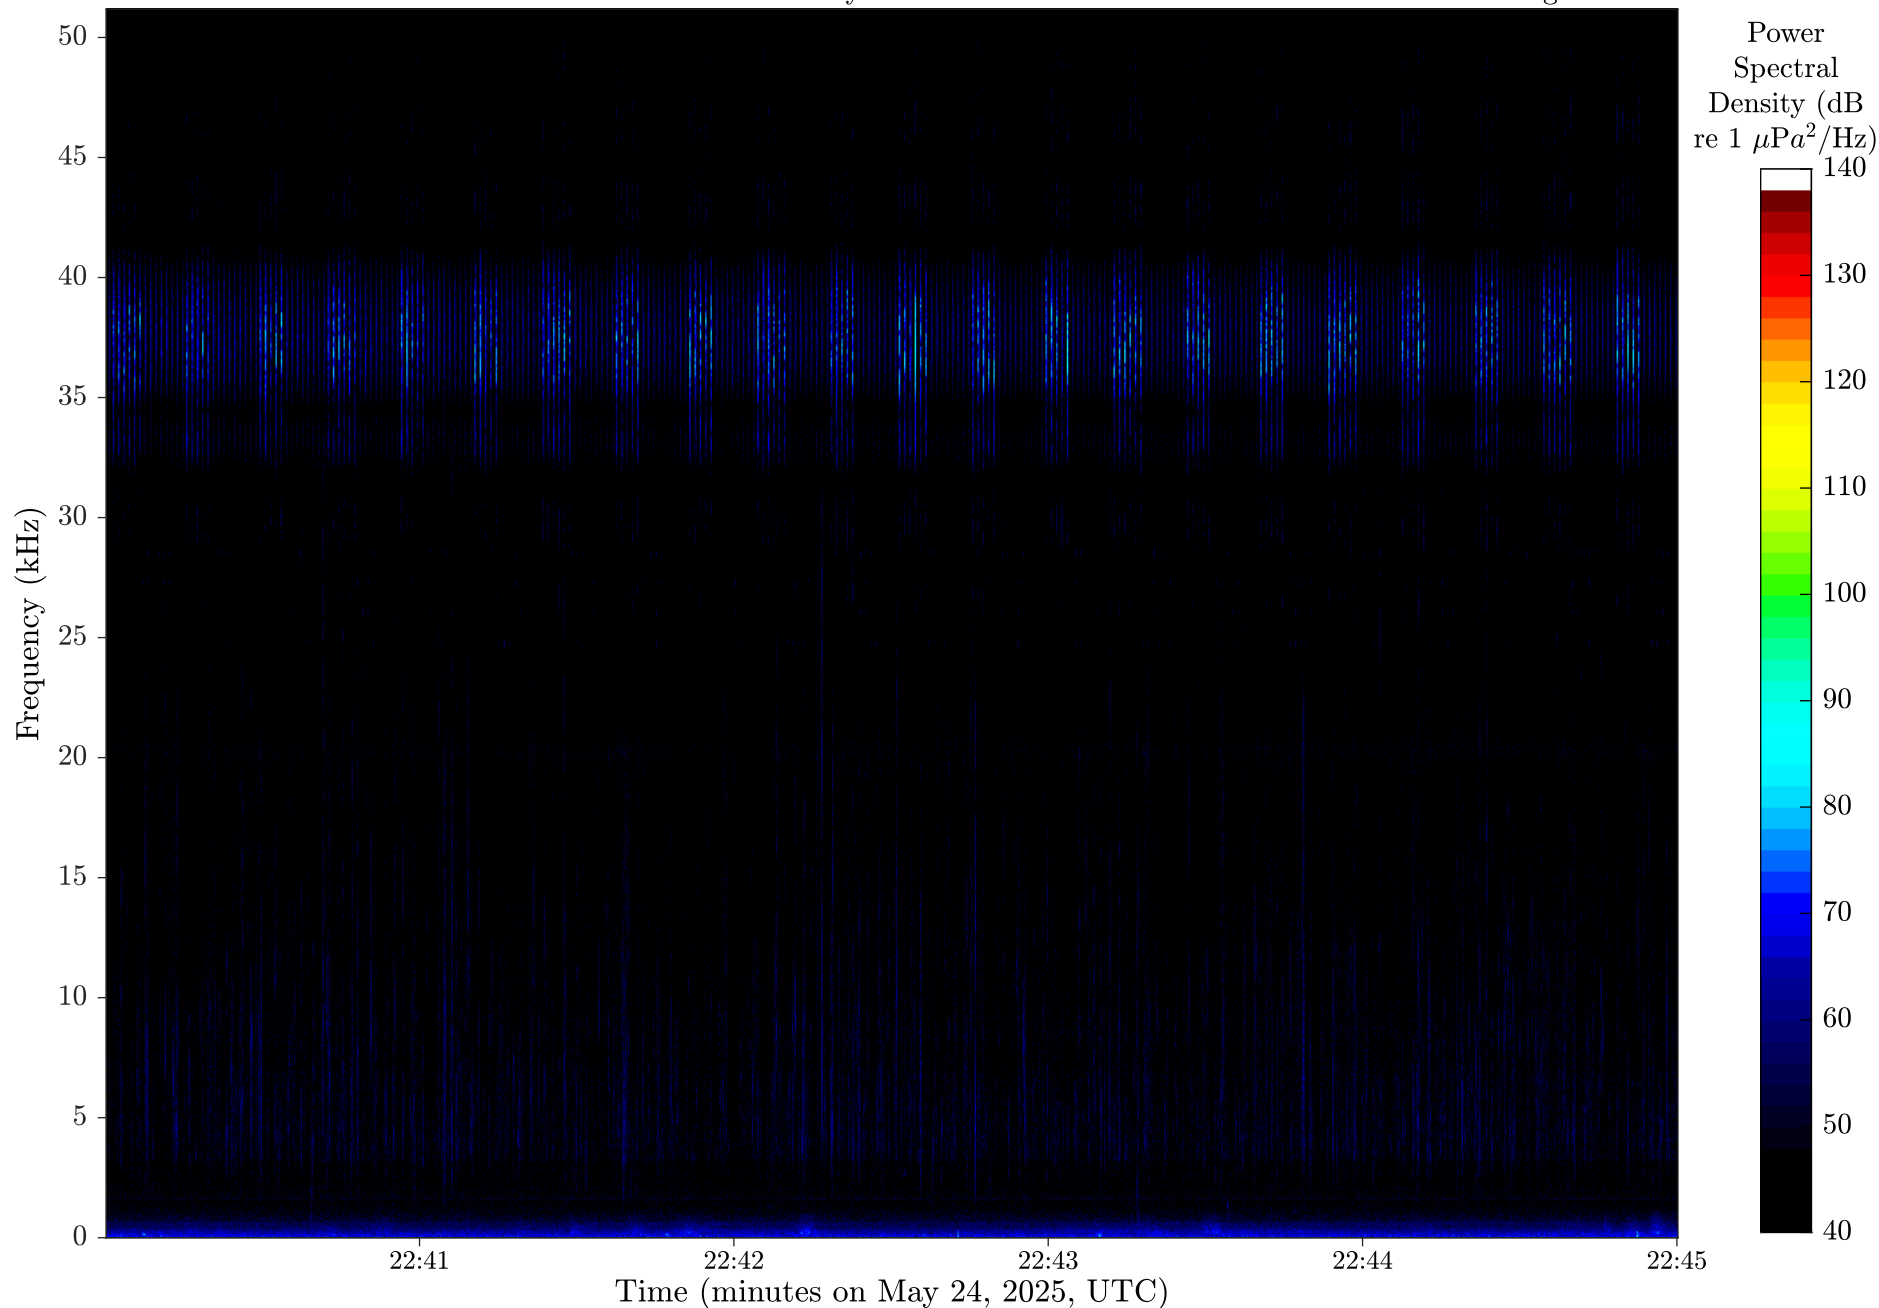


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:55:50 UTC

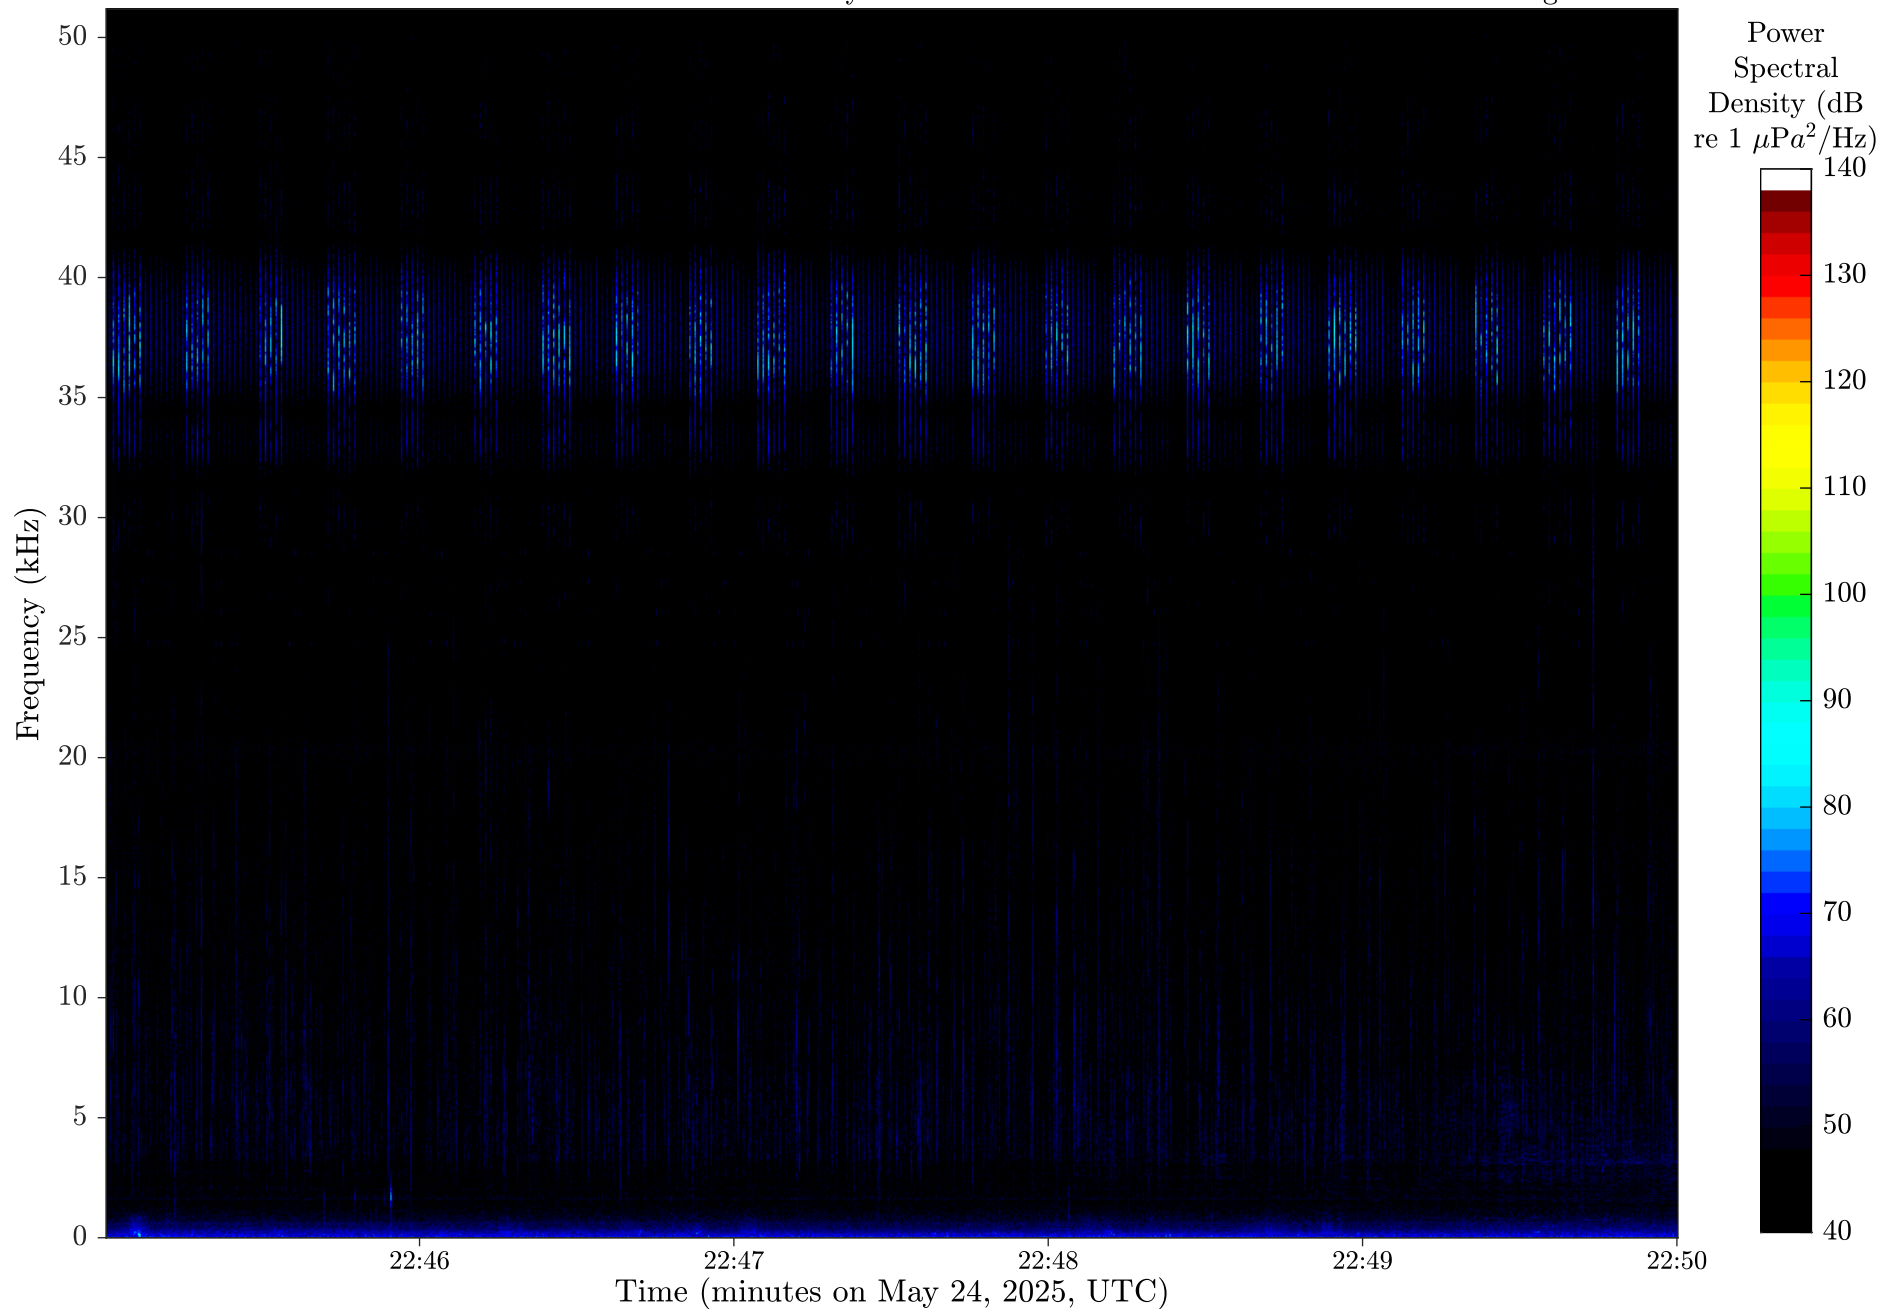

Comments: 34.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:55:58 UTC

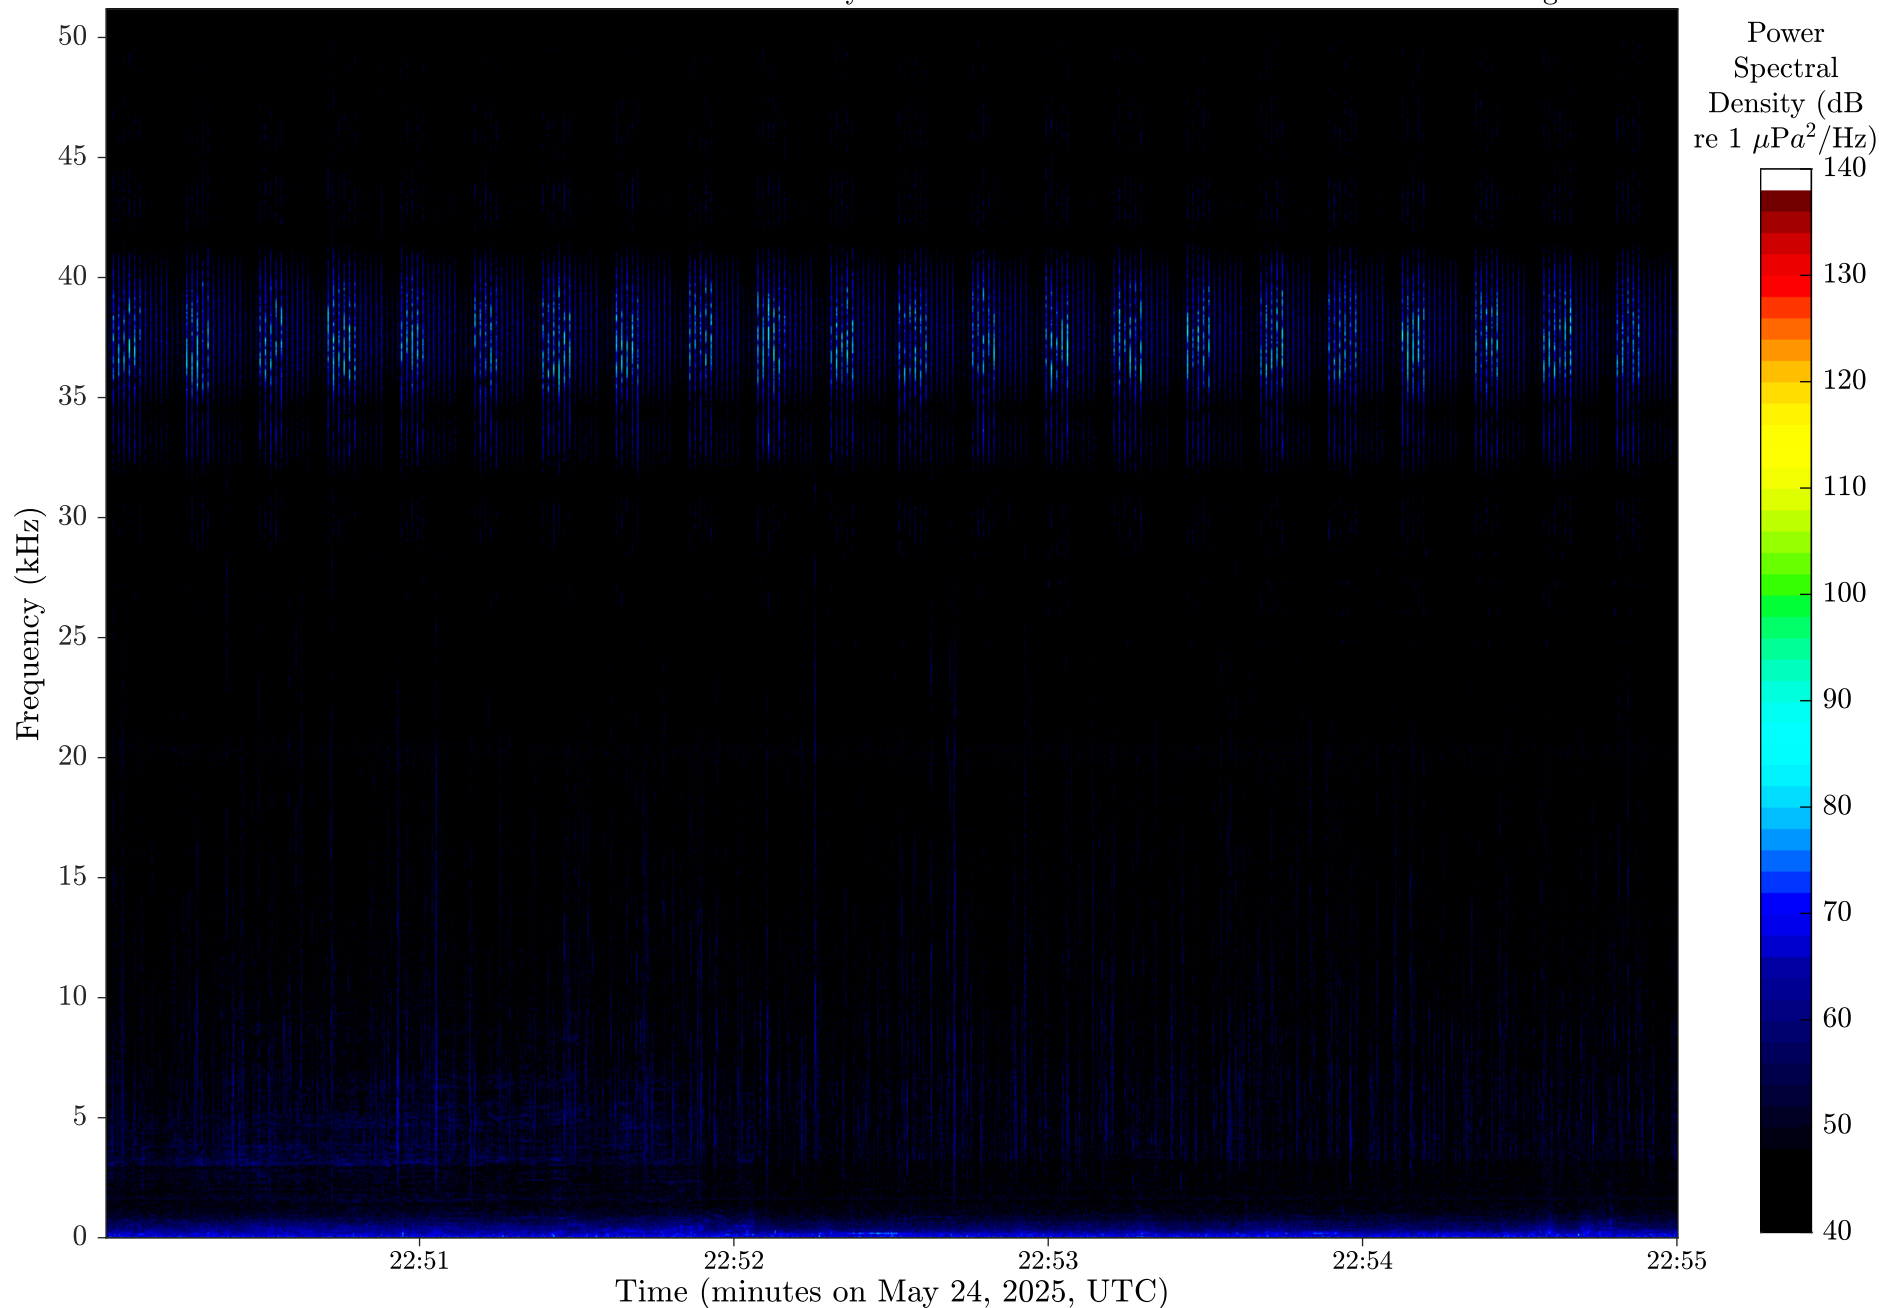


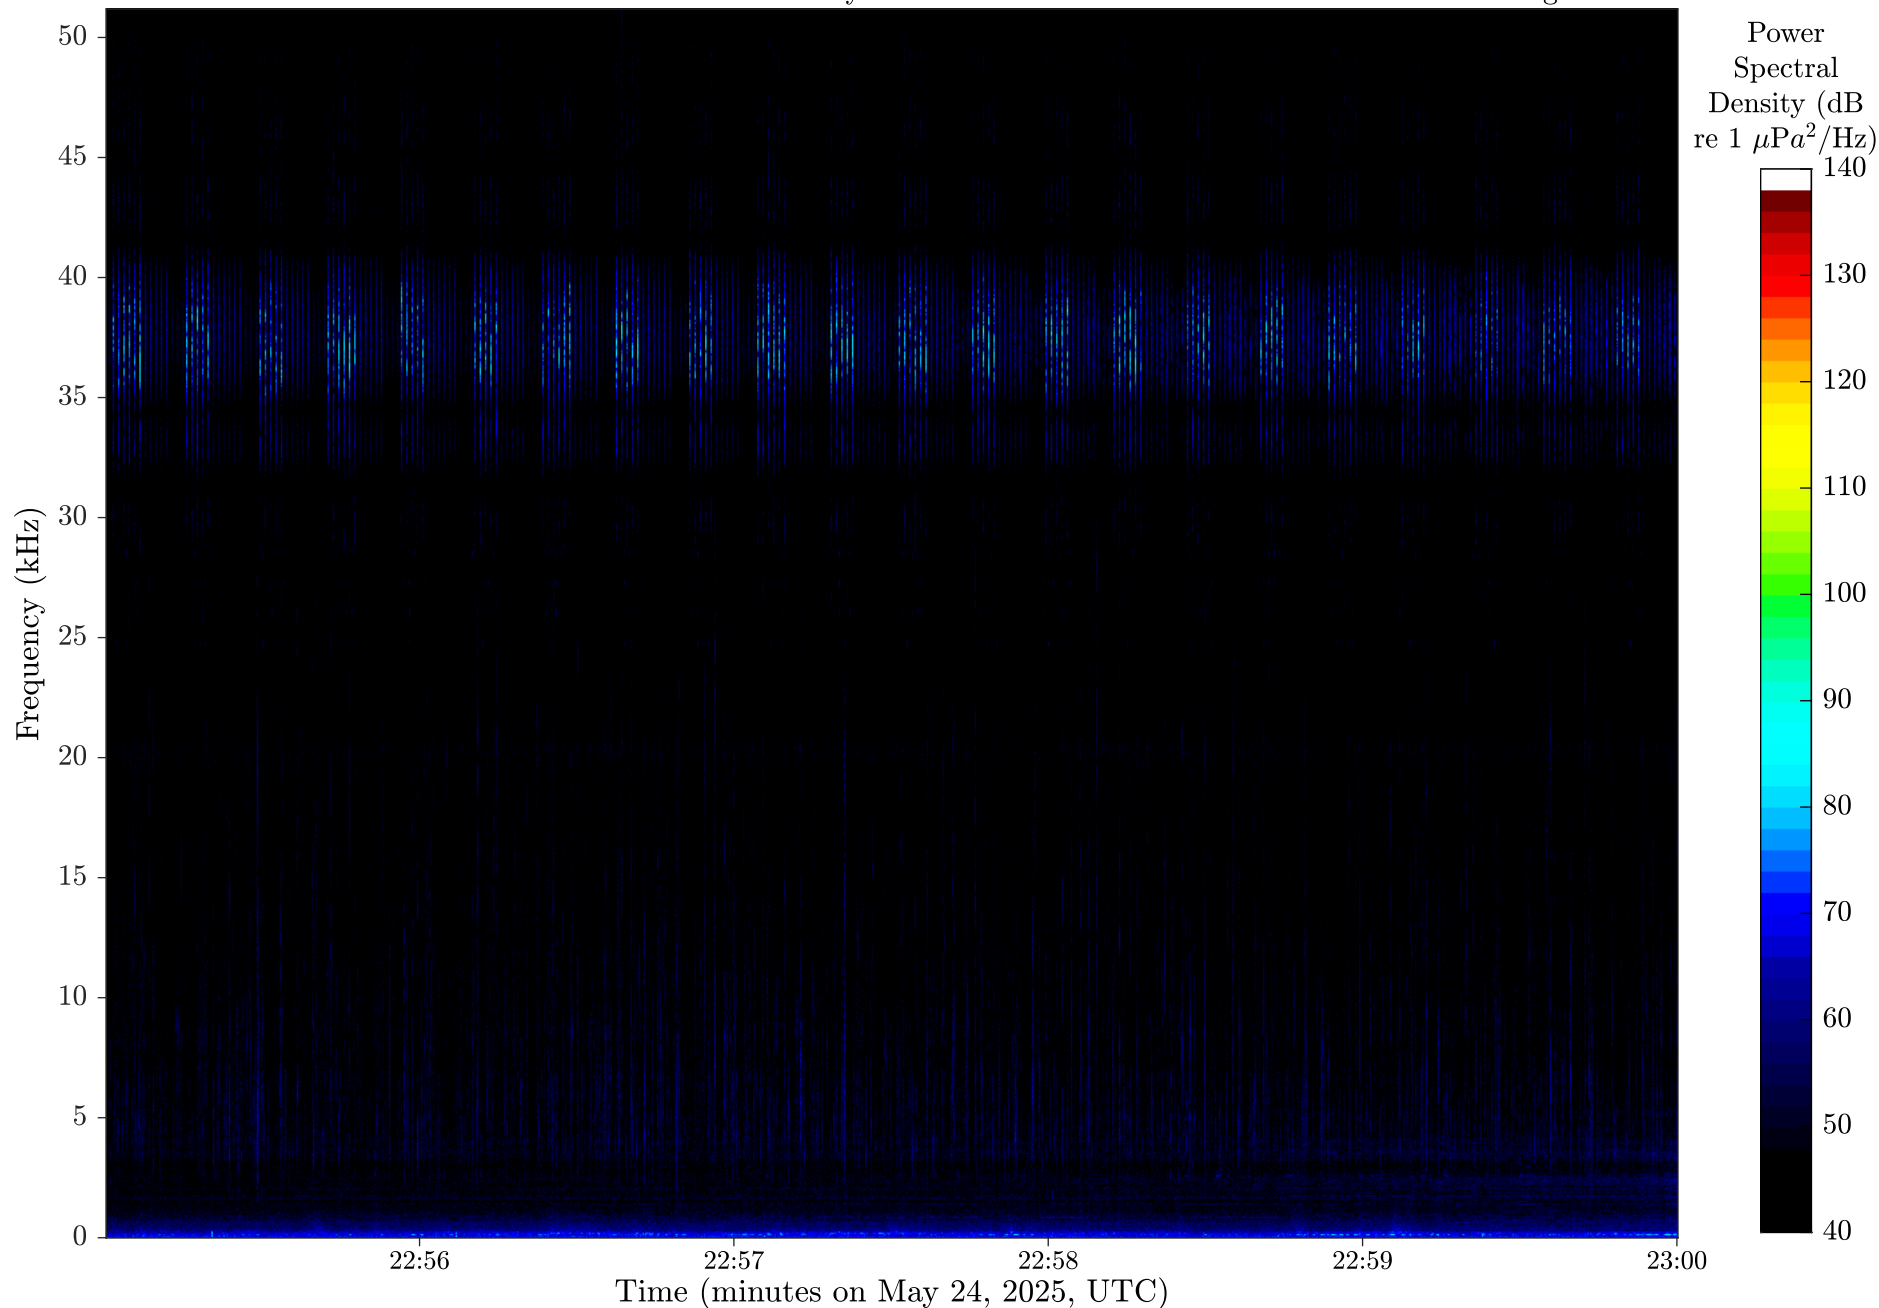

Comments: 34.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:56:13 UTC

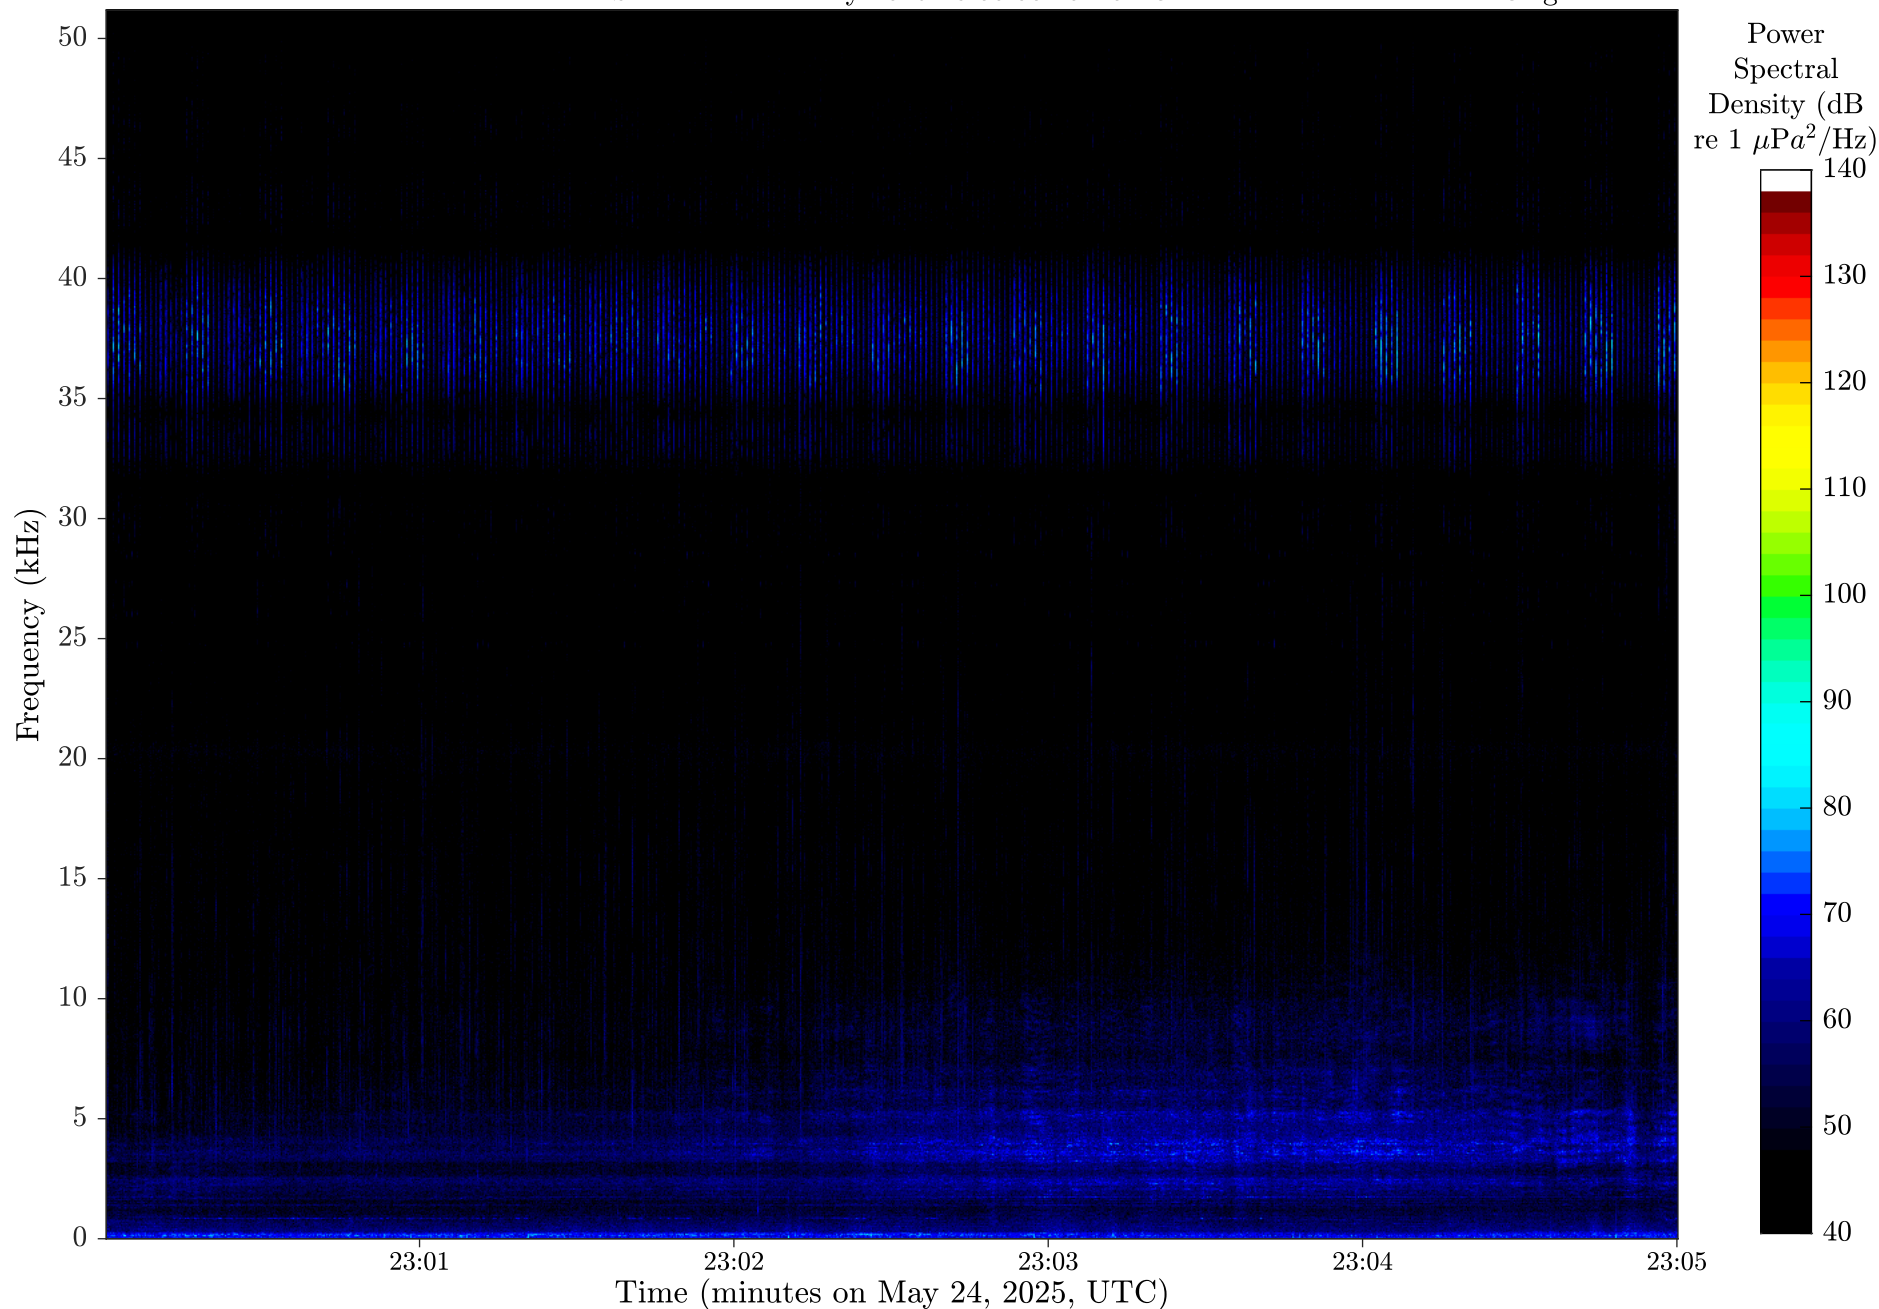

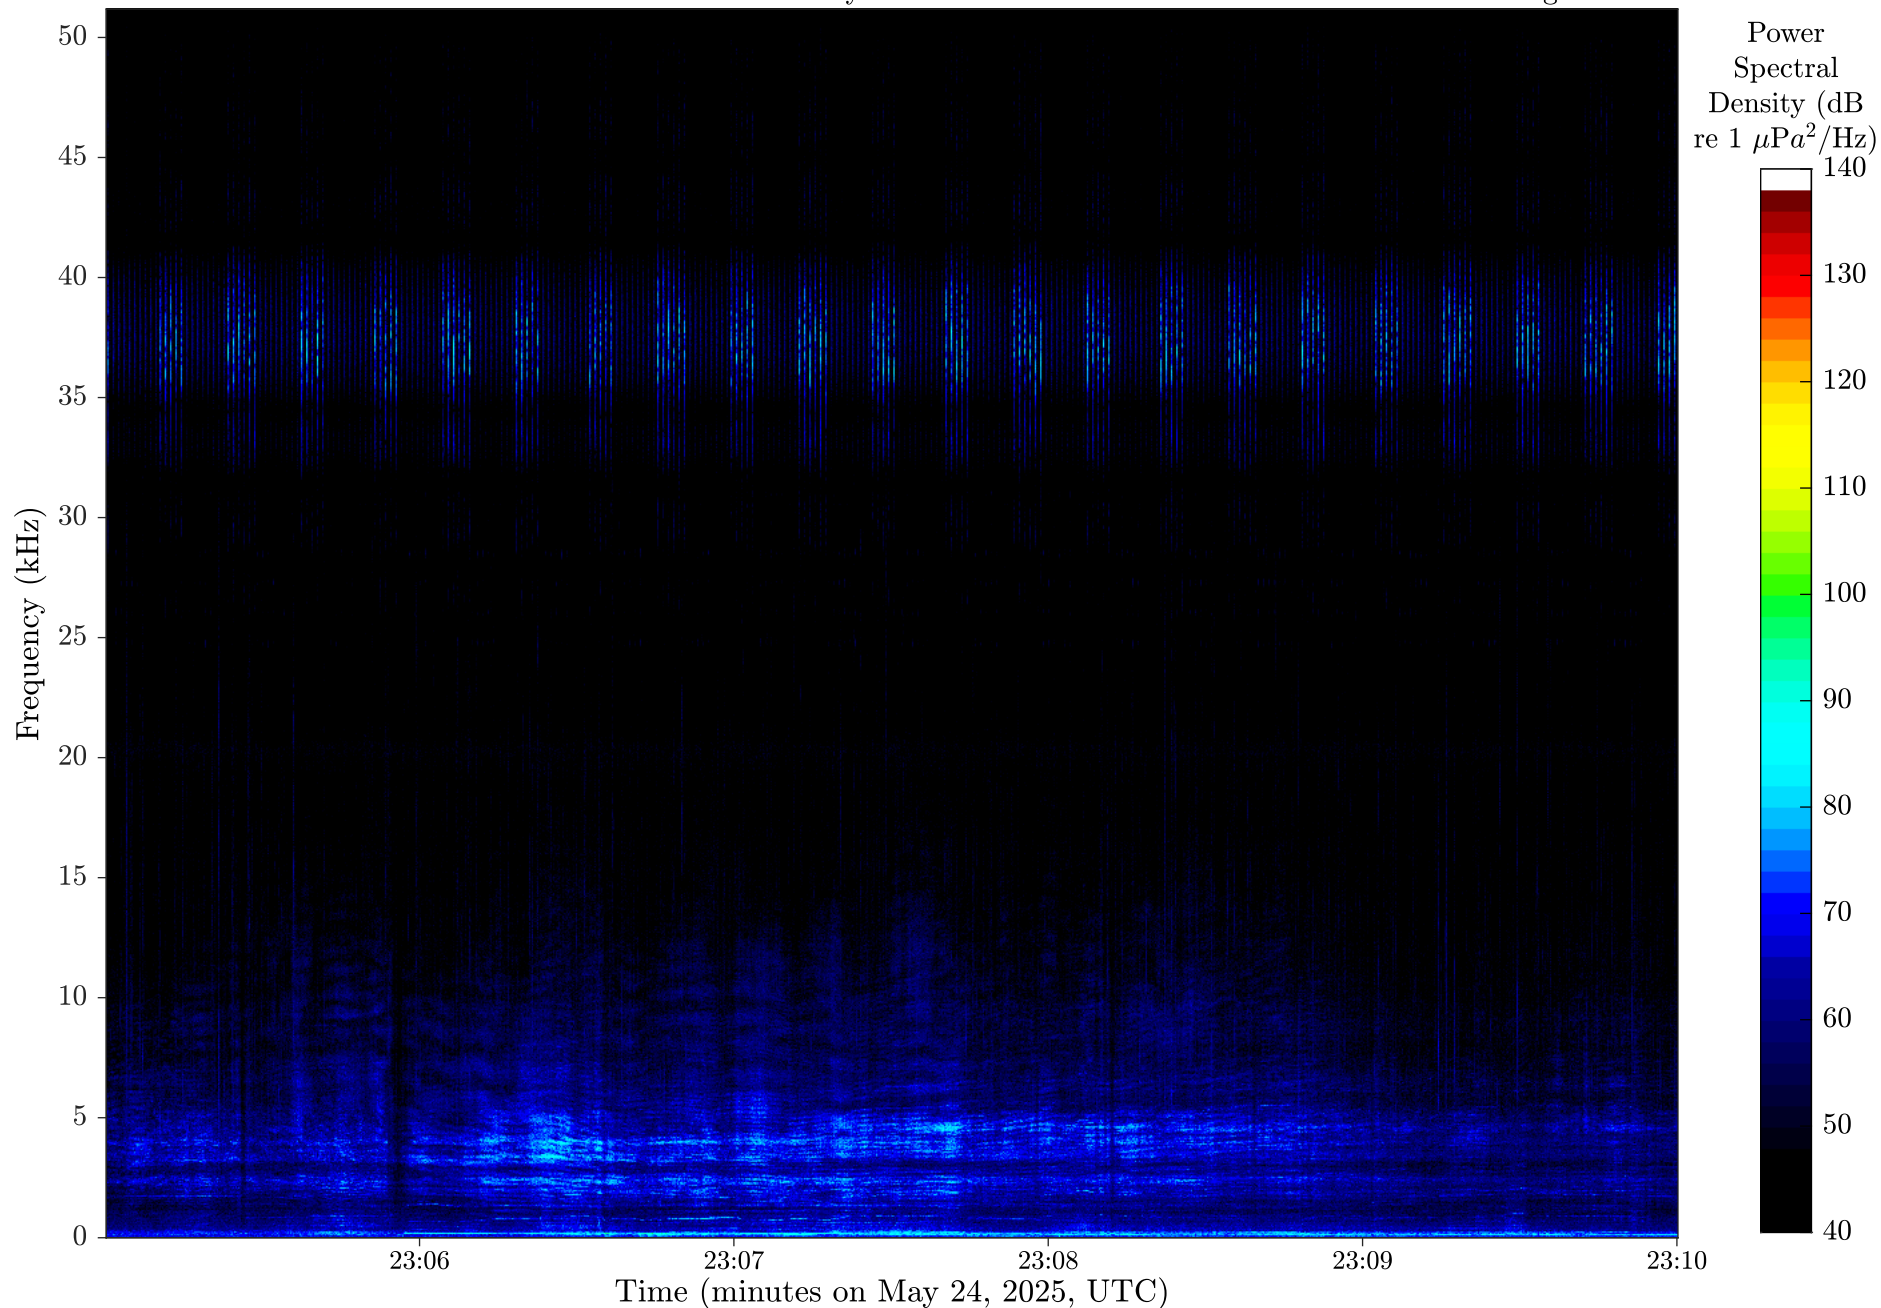


Comments: 31.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:56:27 UTC

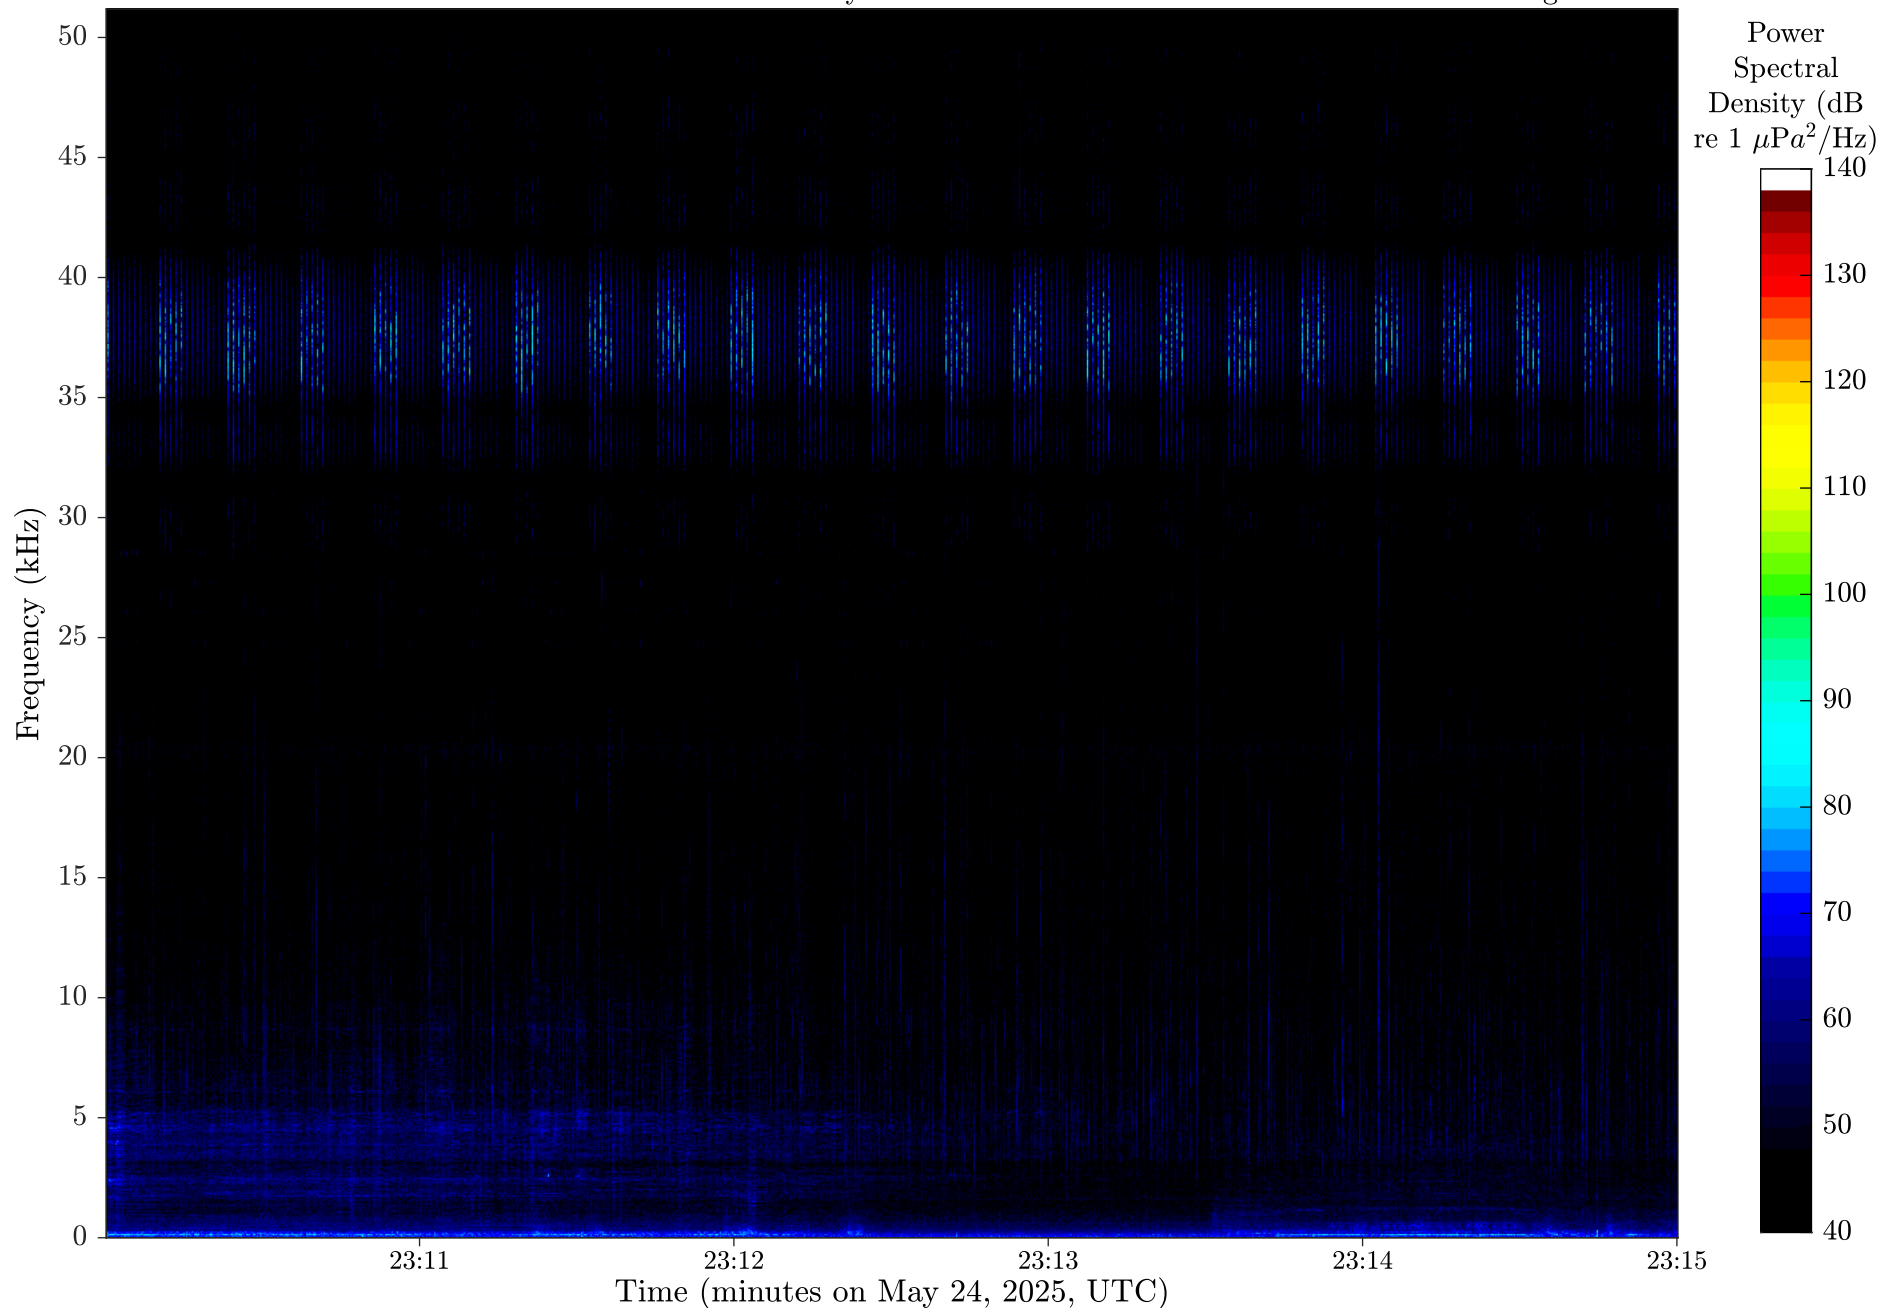


Comments: 33.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:56:36 UTC

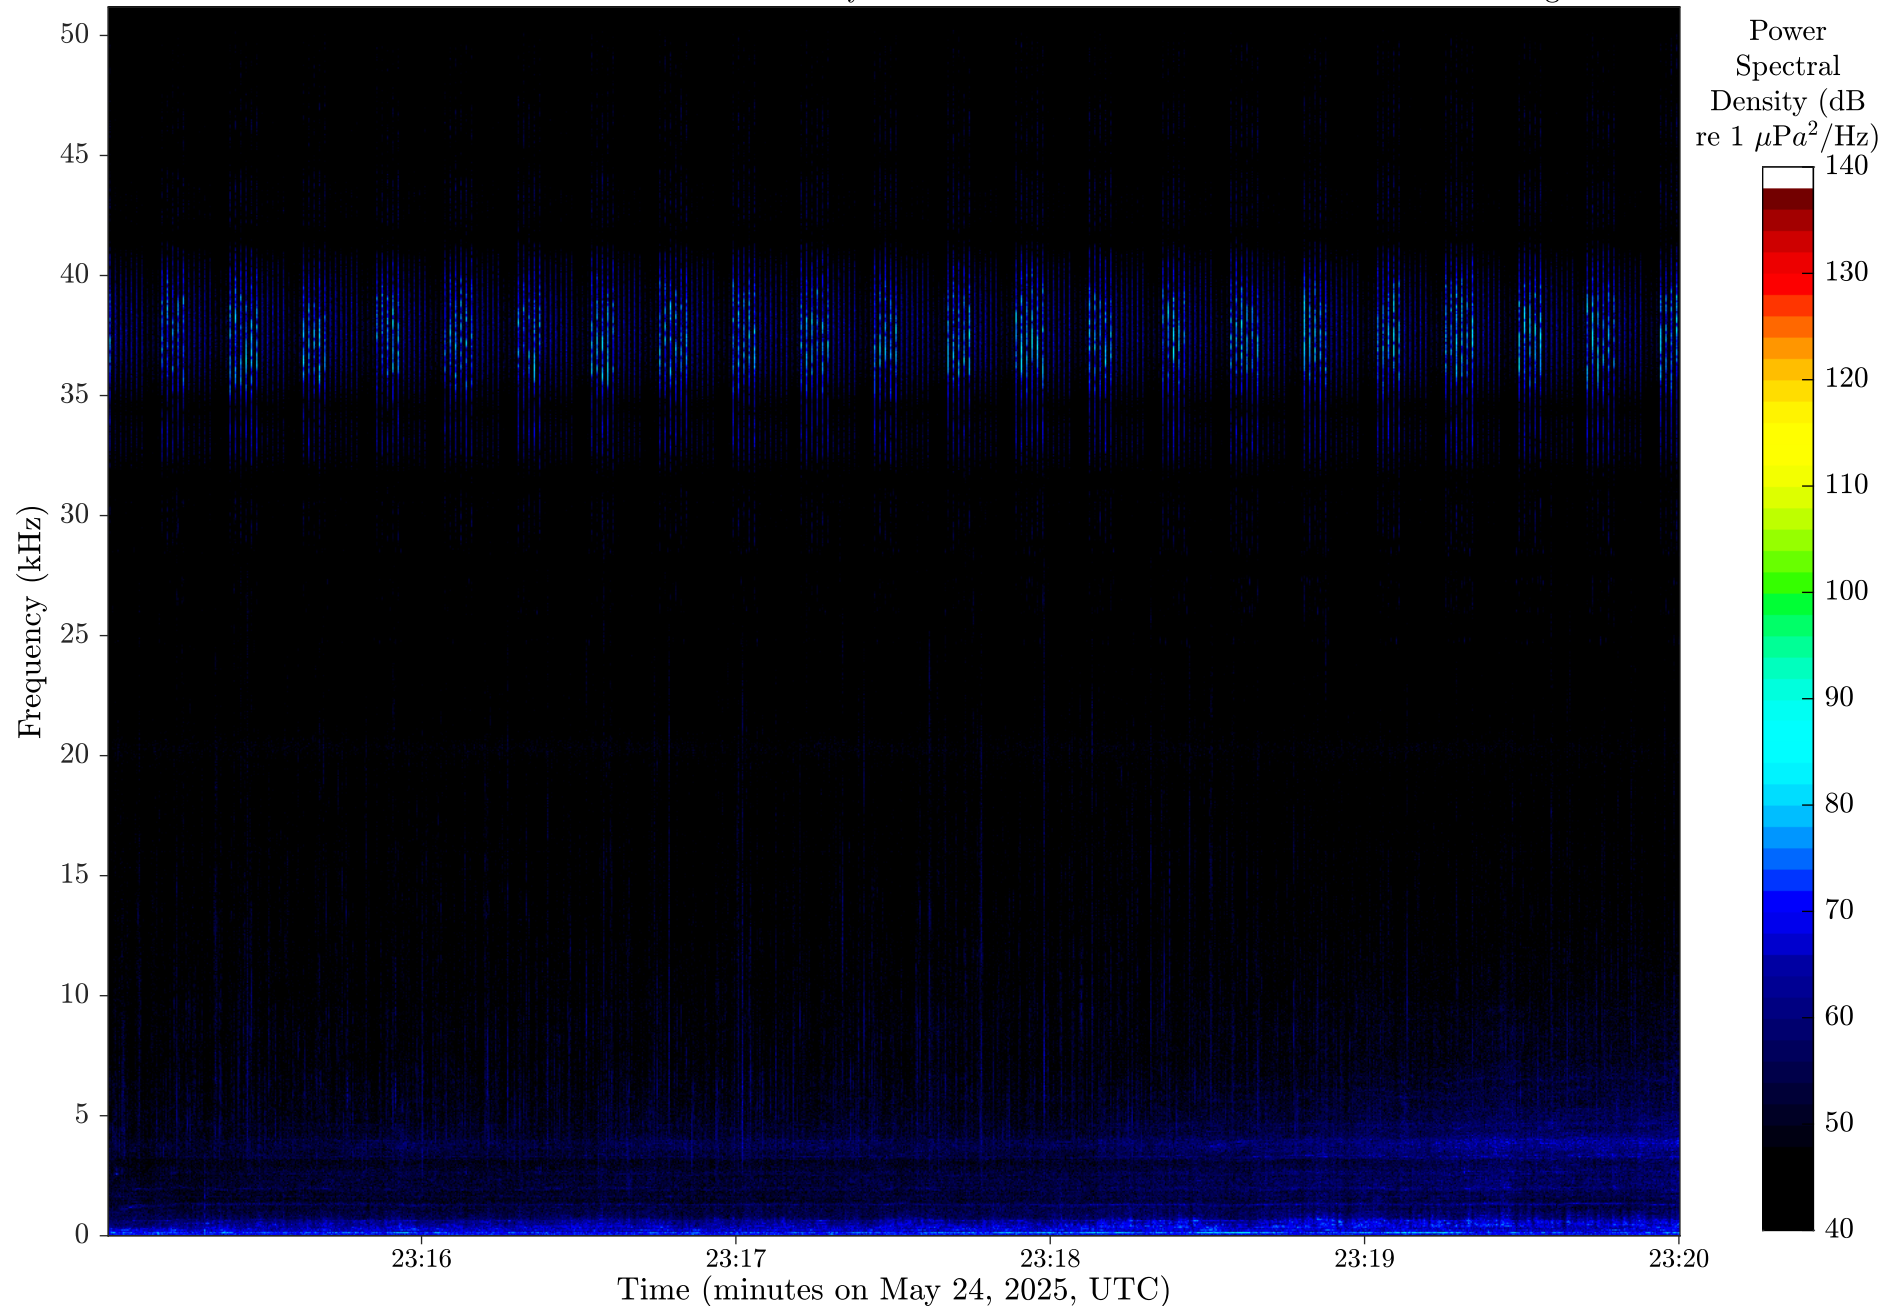


Comments: 33.6 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.


Plot generated 26-Nov-2025 11:56:44 UTC

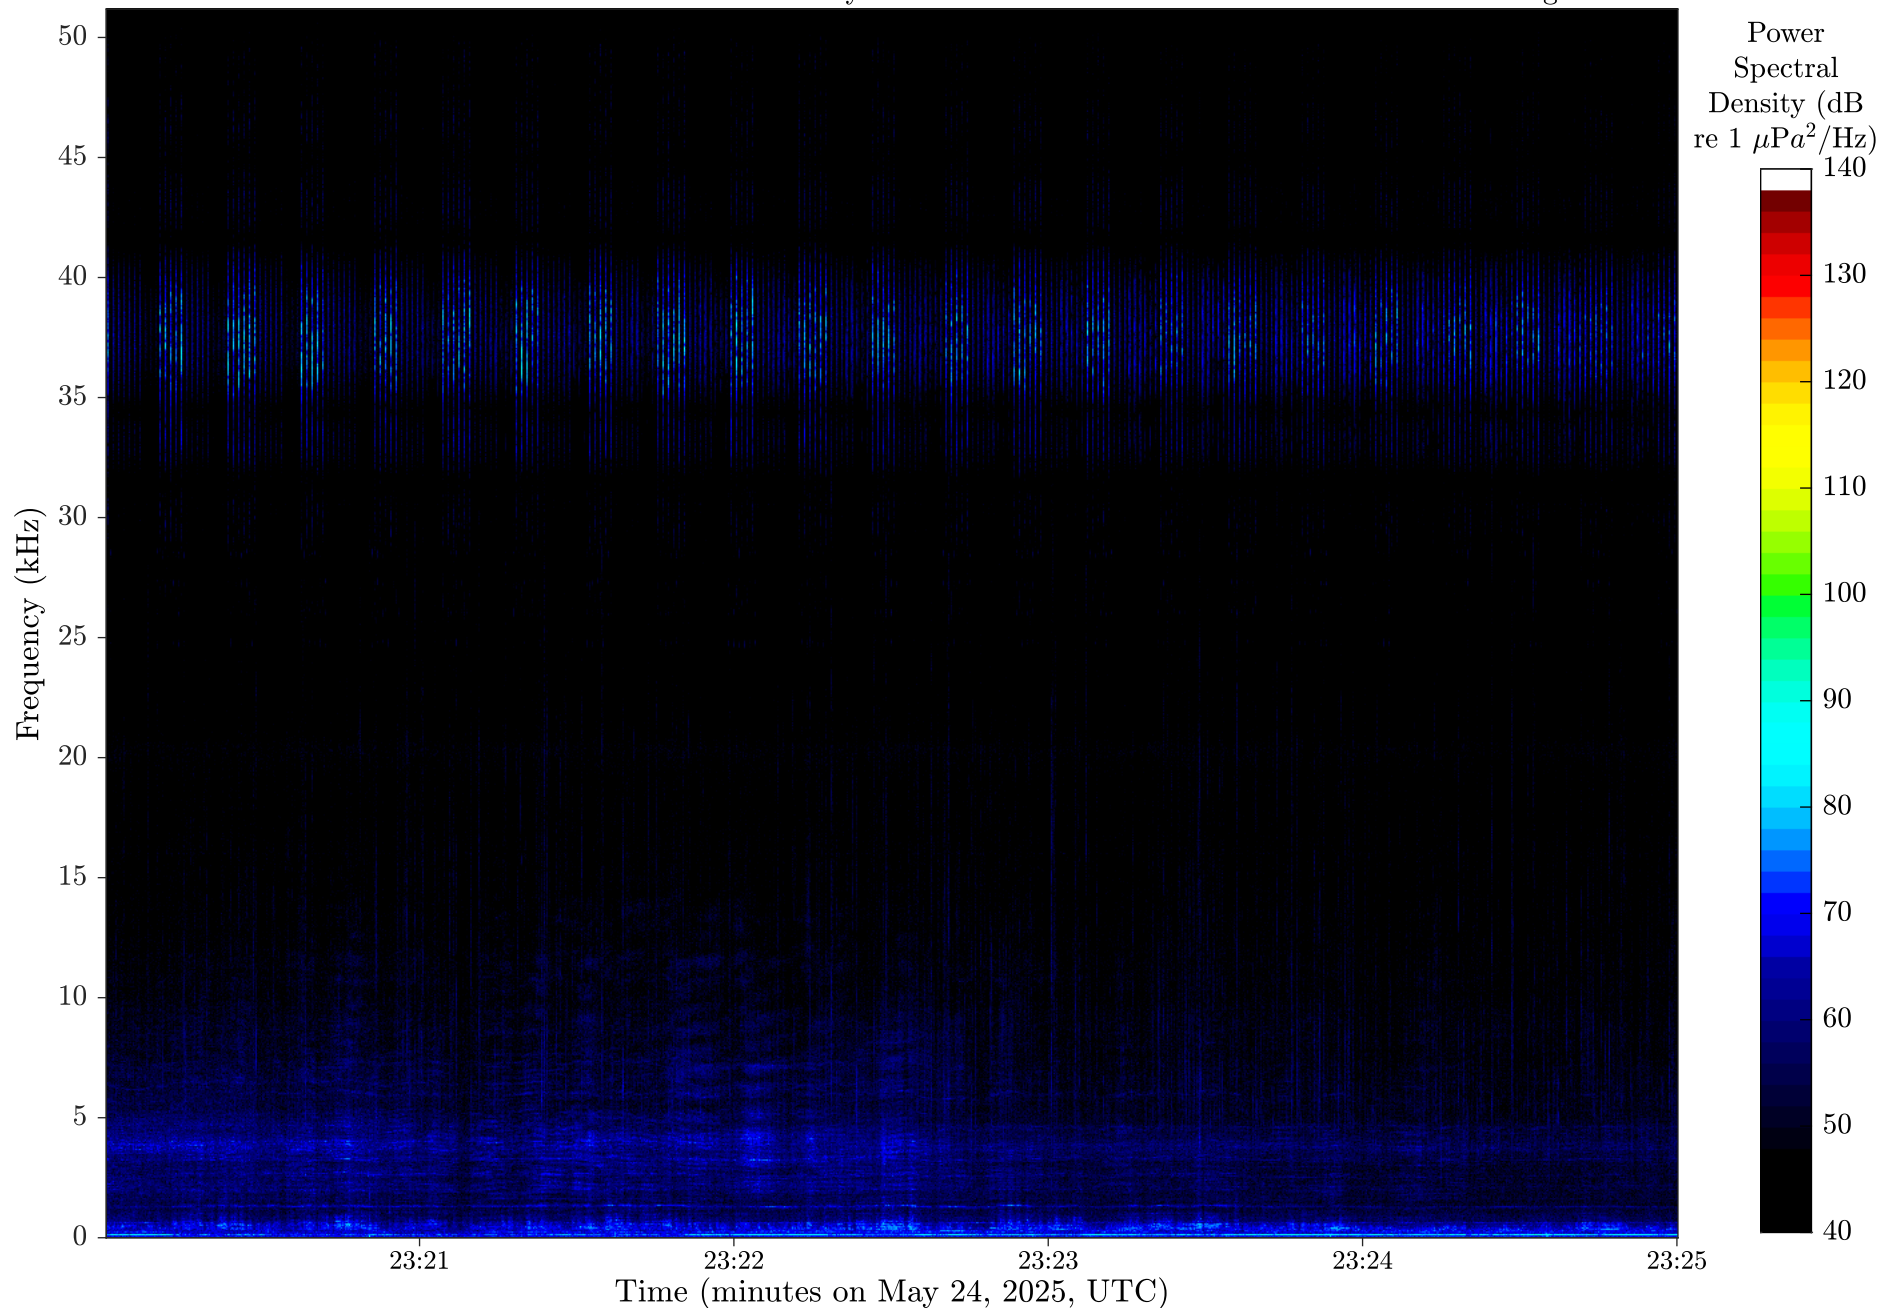



Comments: 30.9 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:56:51 UTC

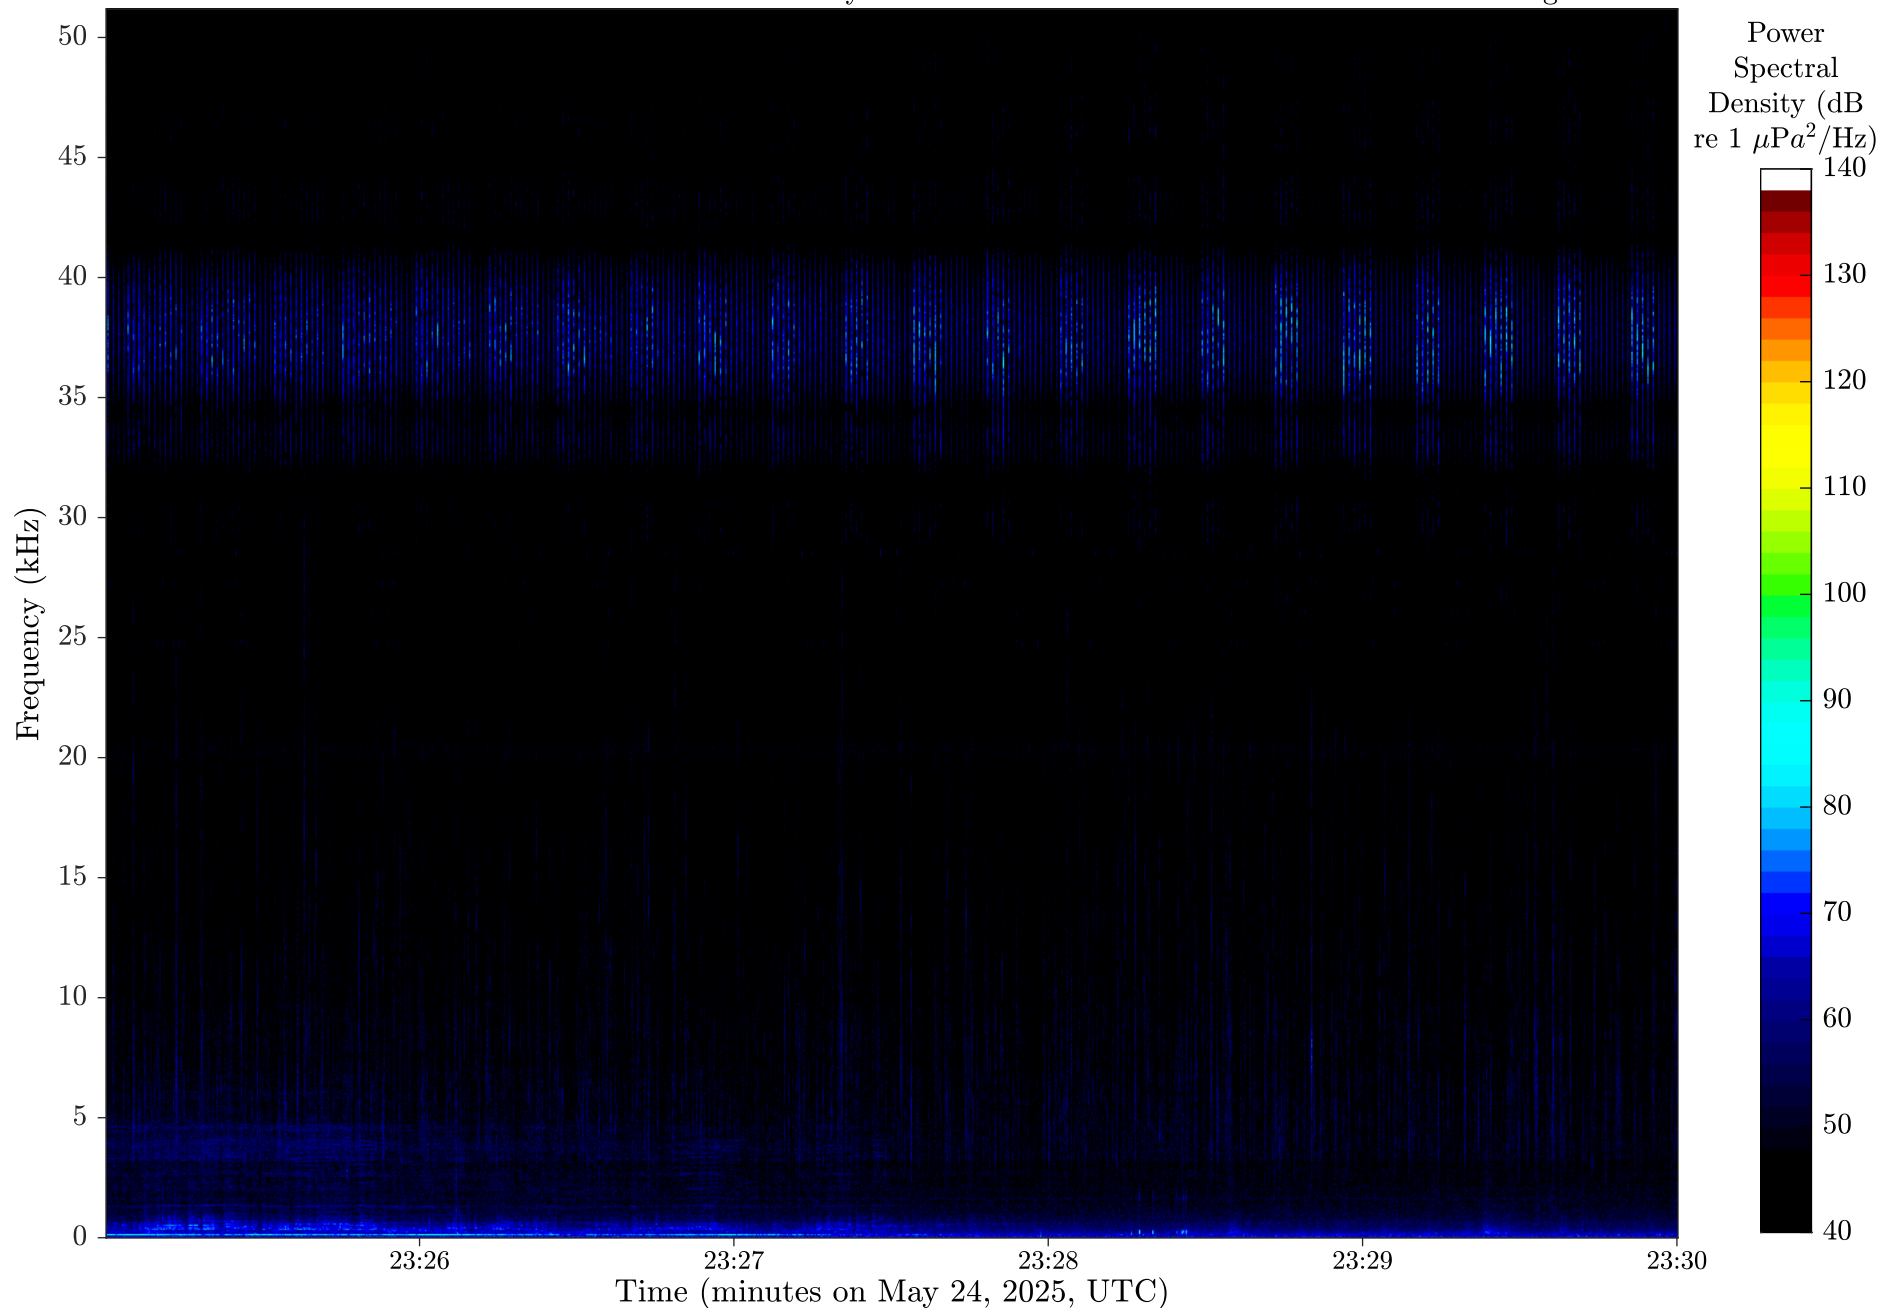

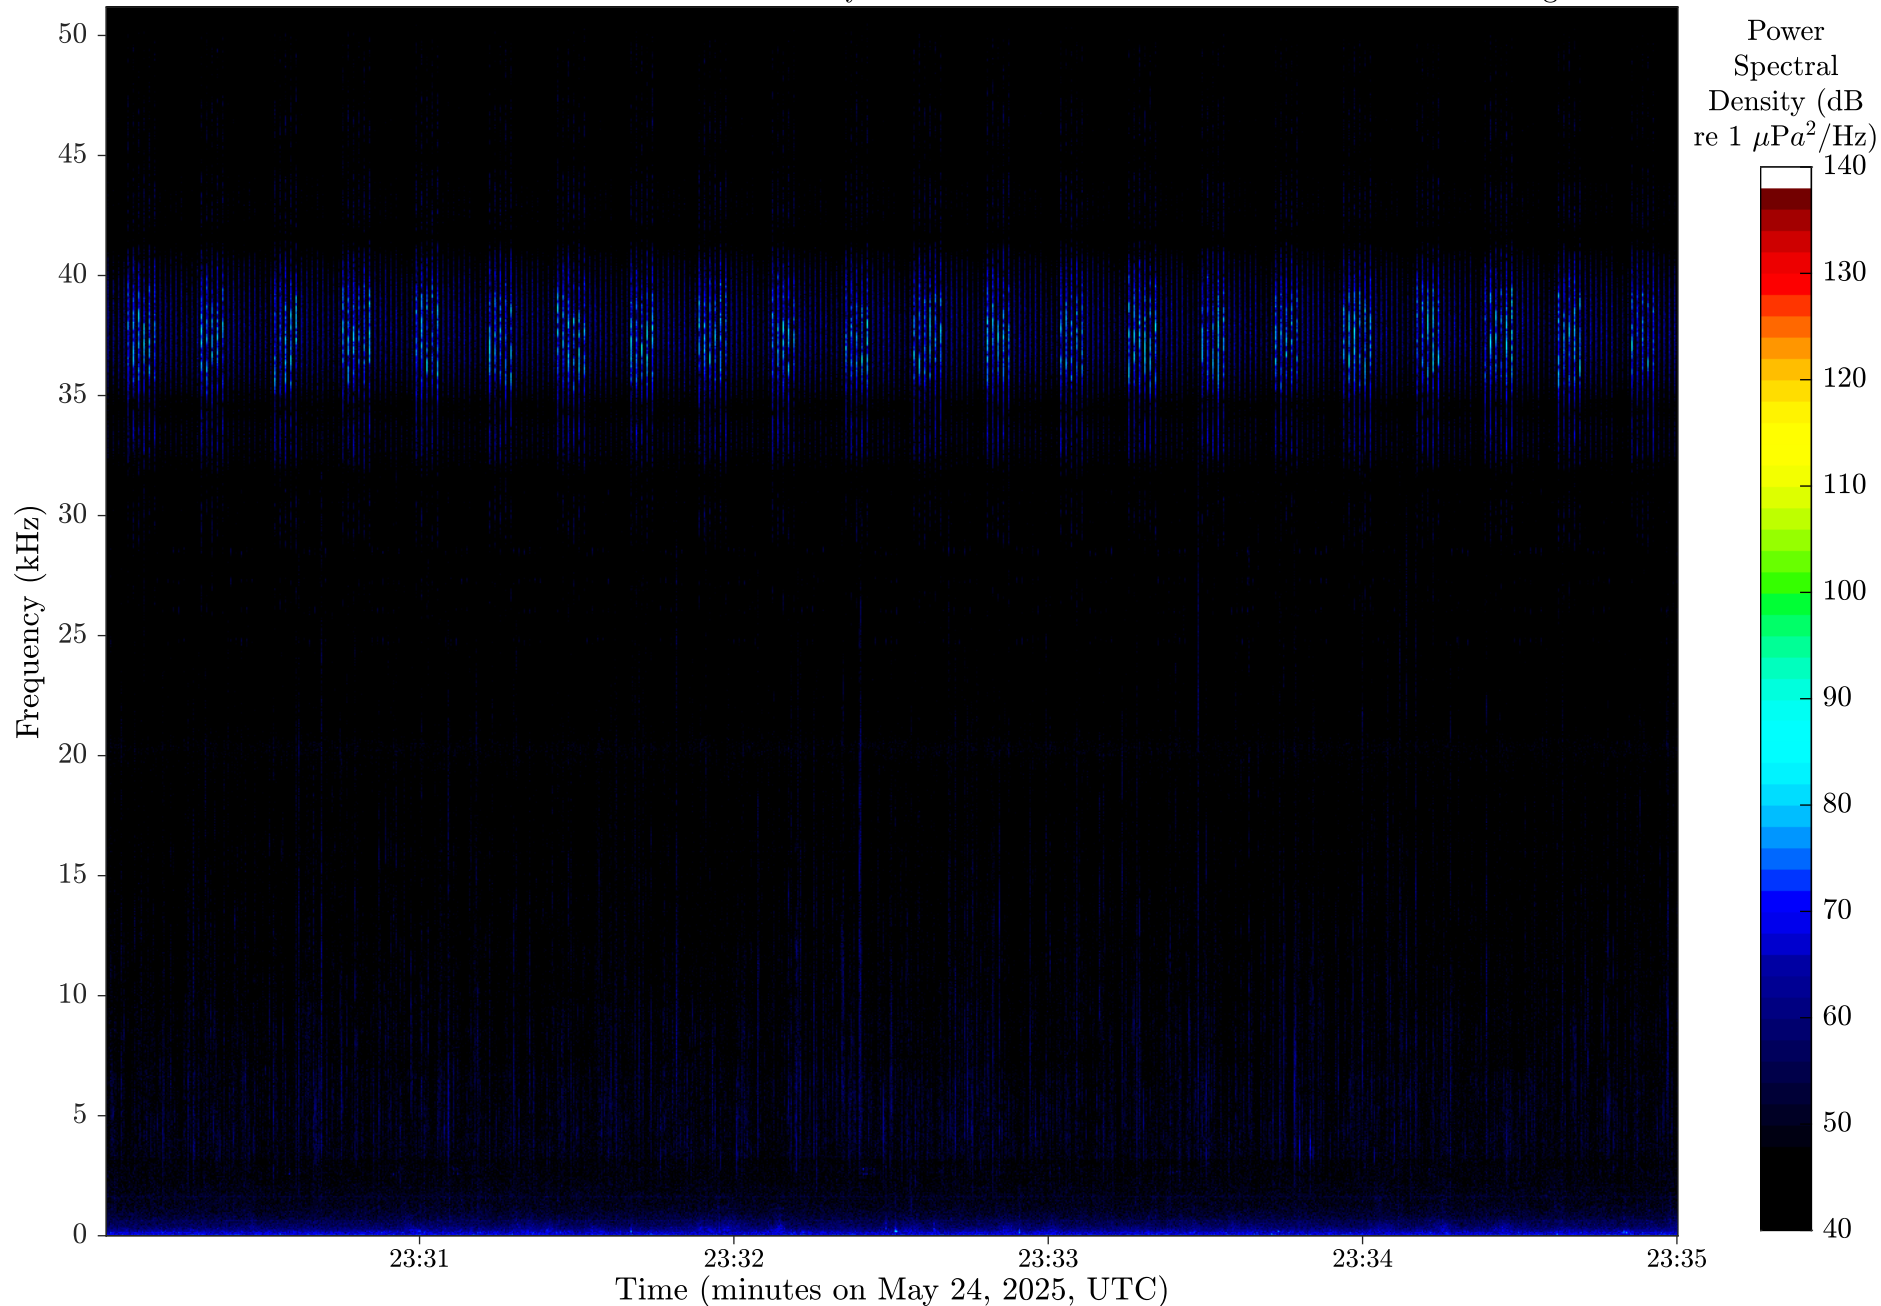


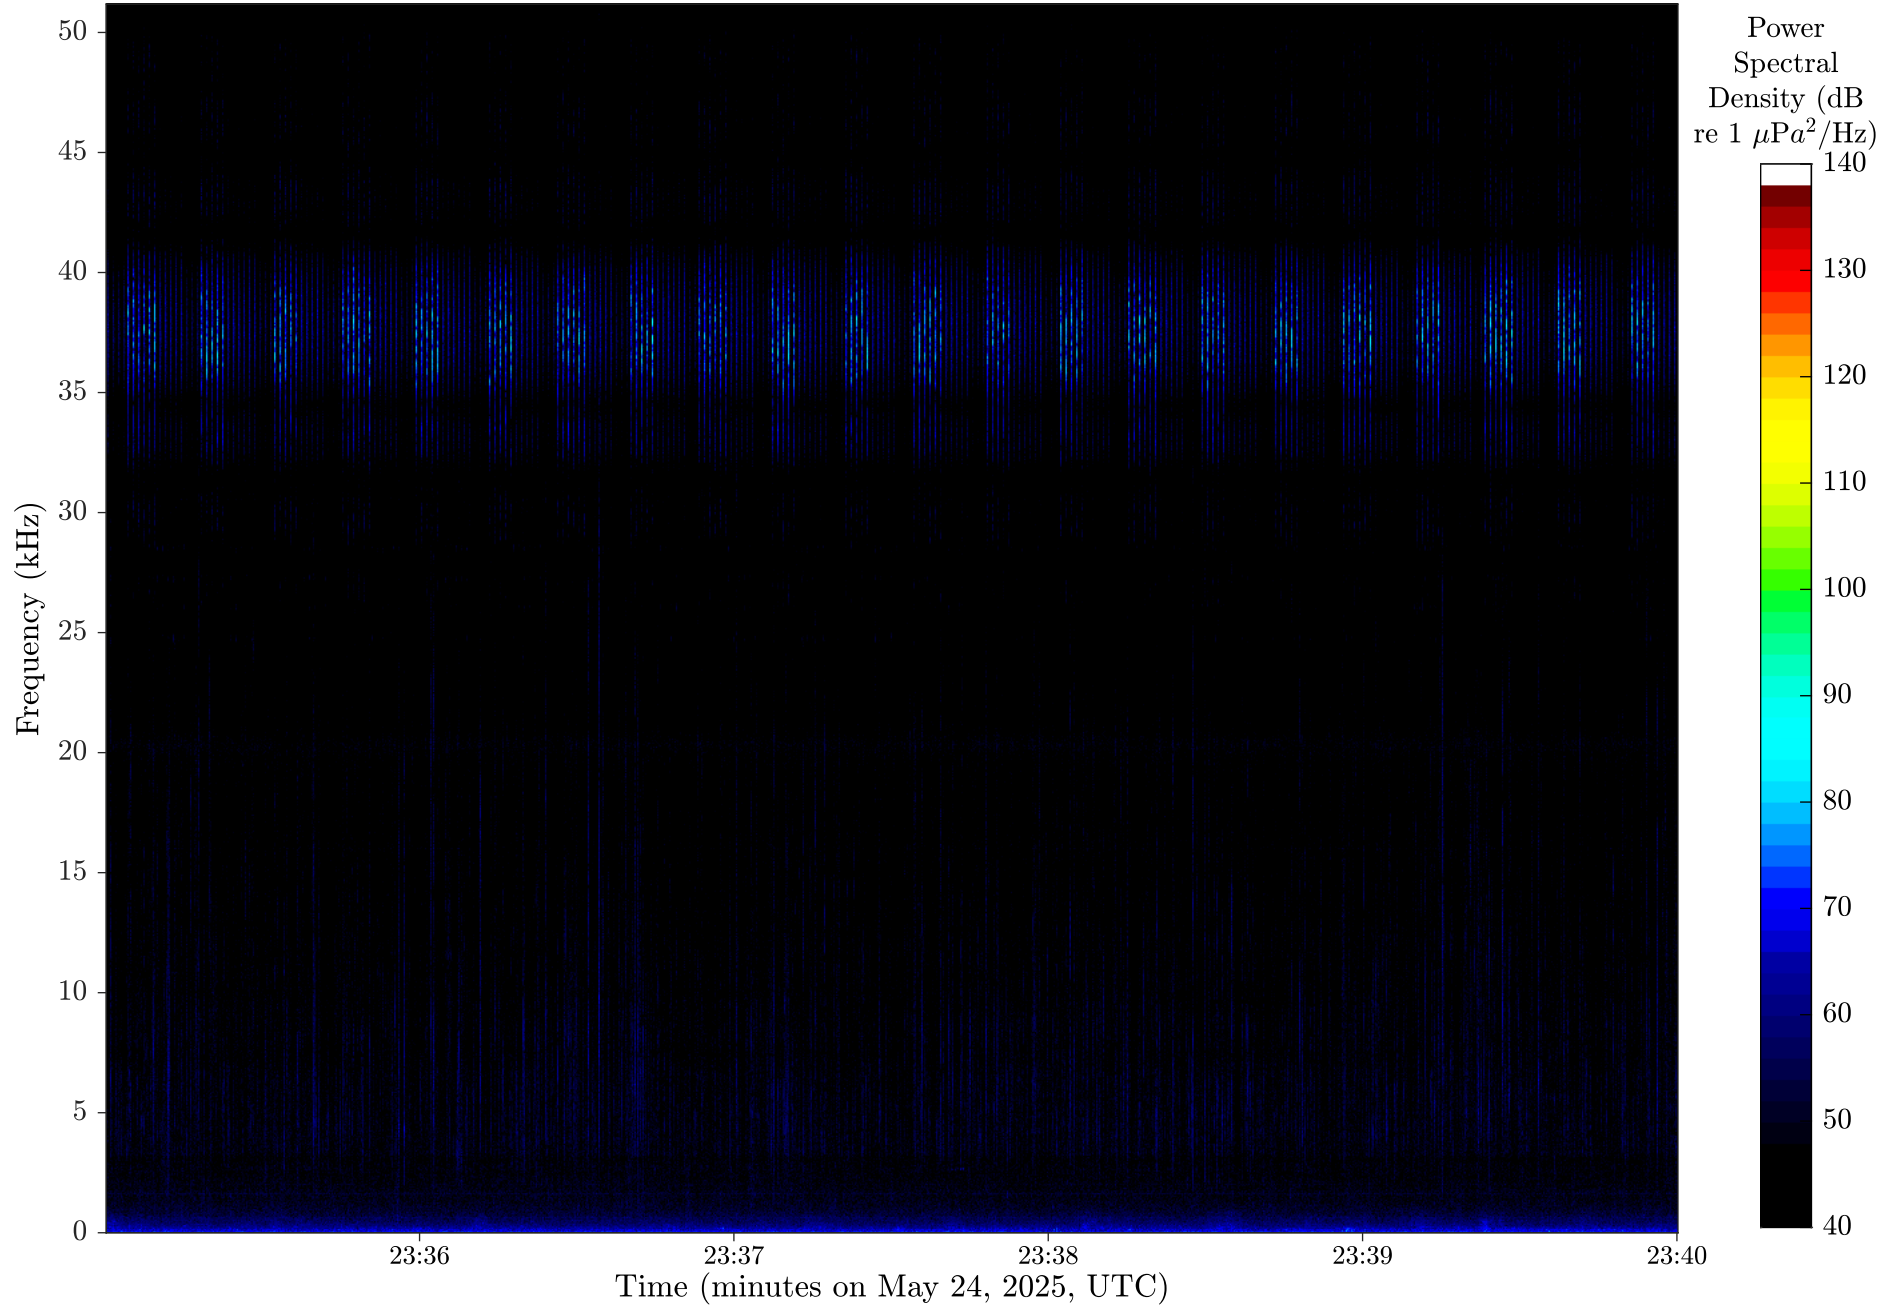

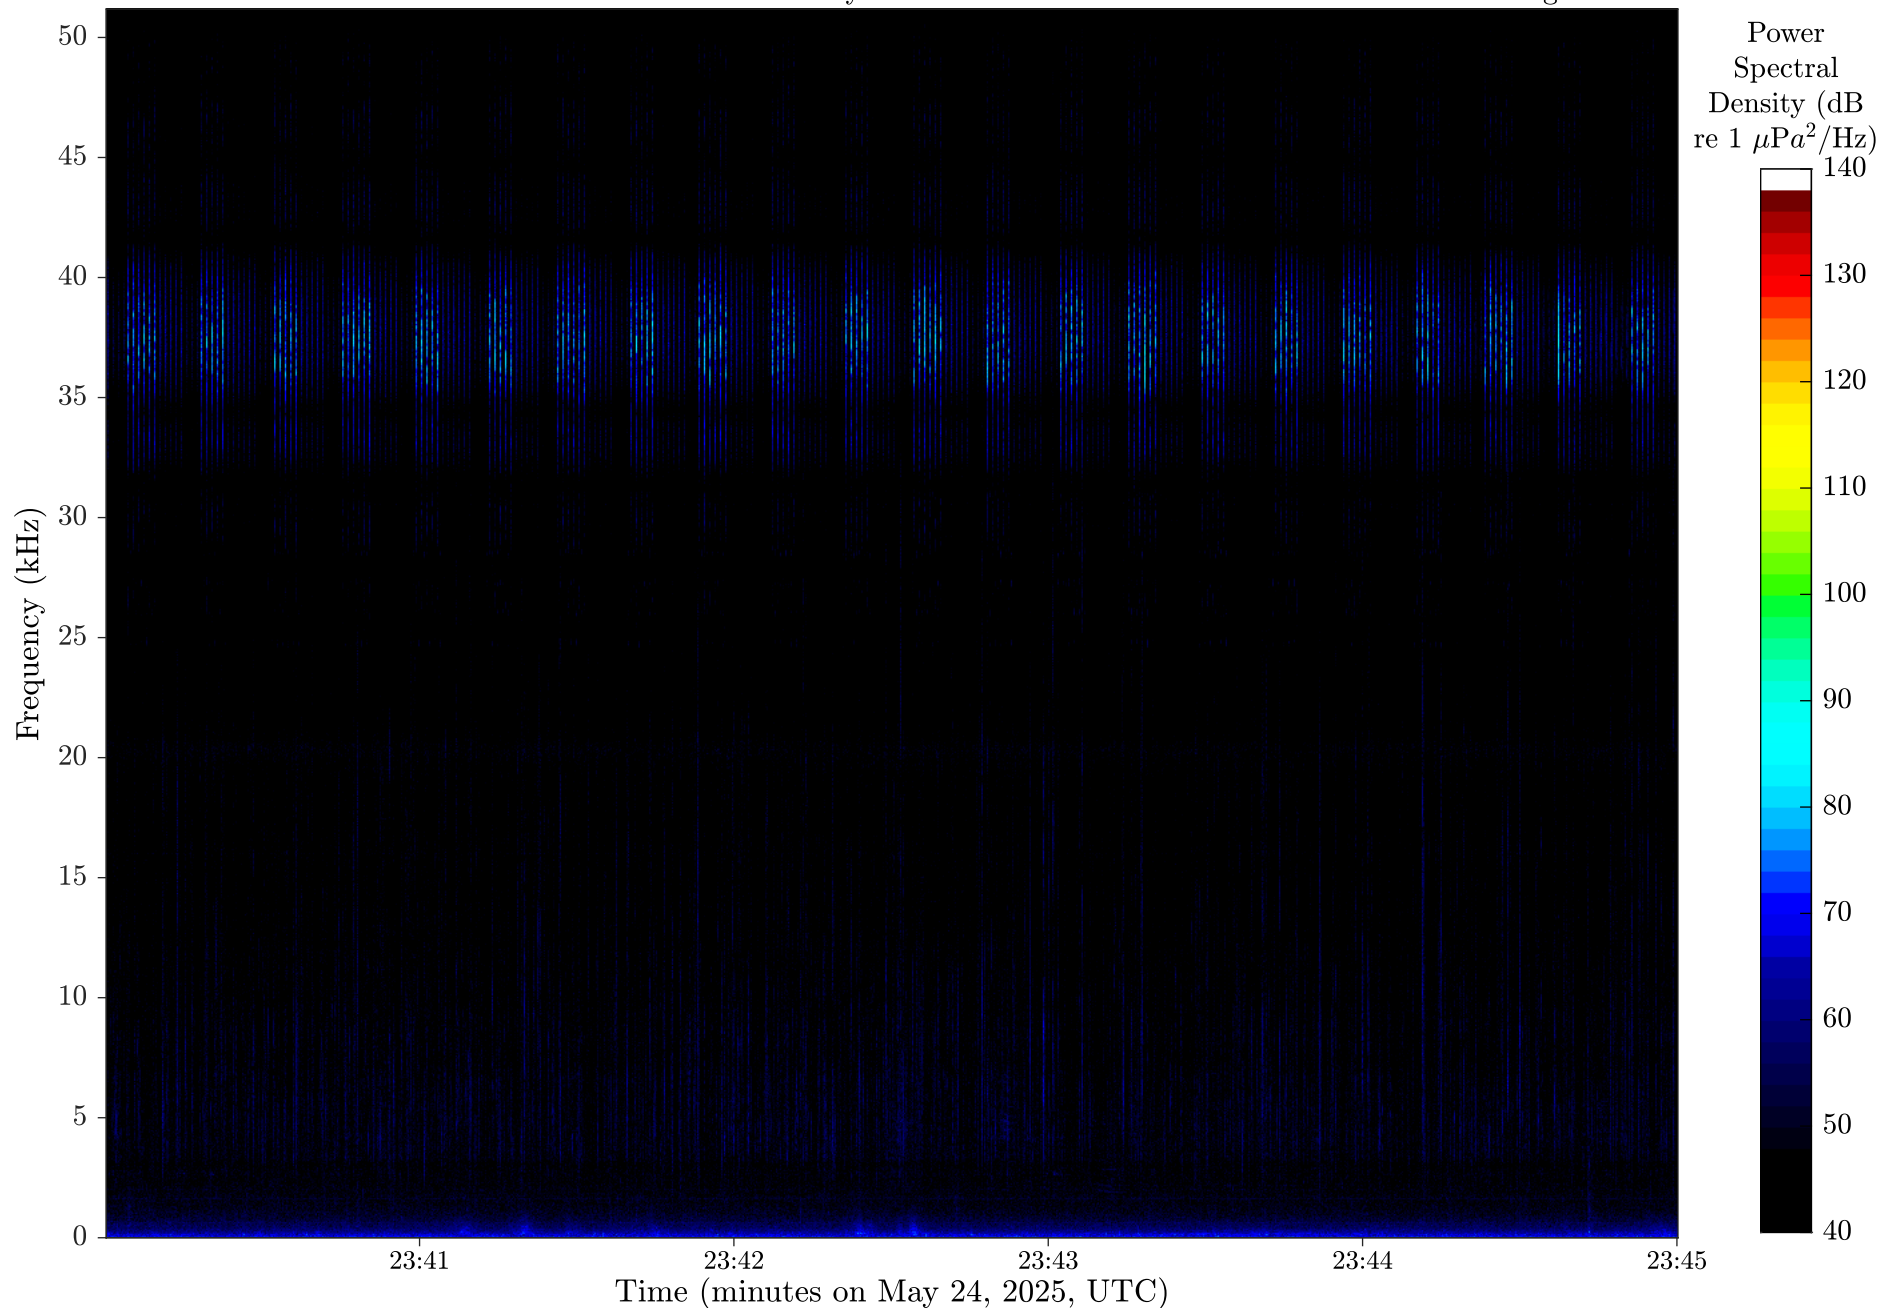


Comments: 35.3 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:57:20 UTC

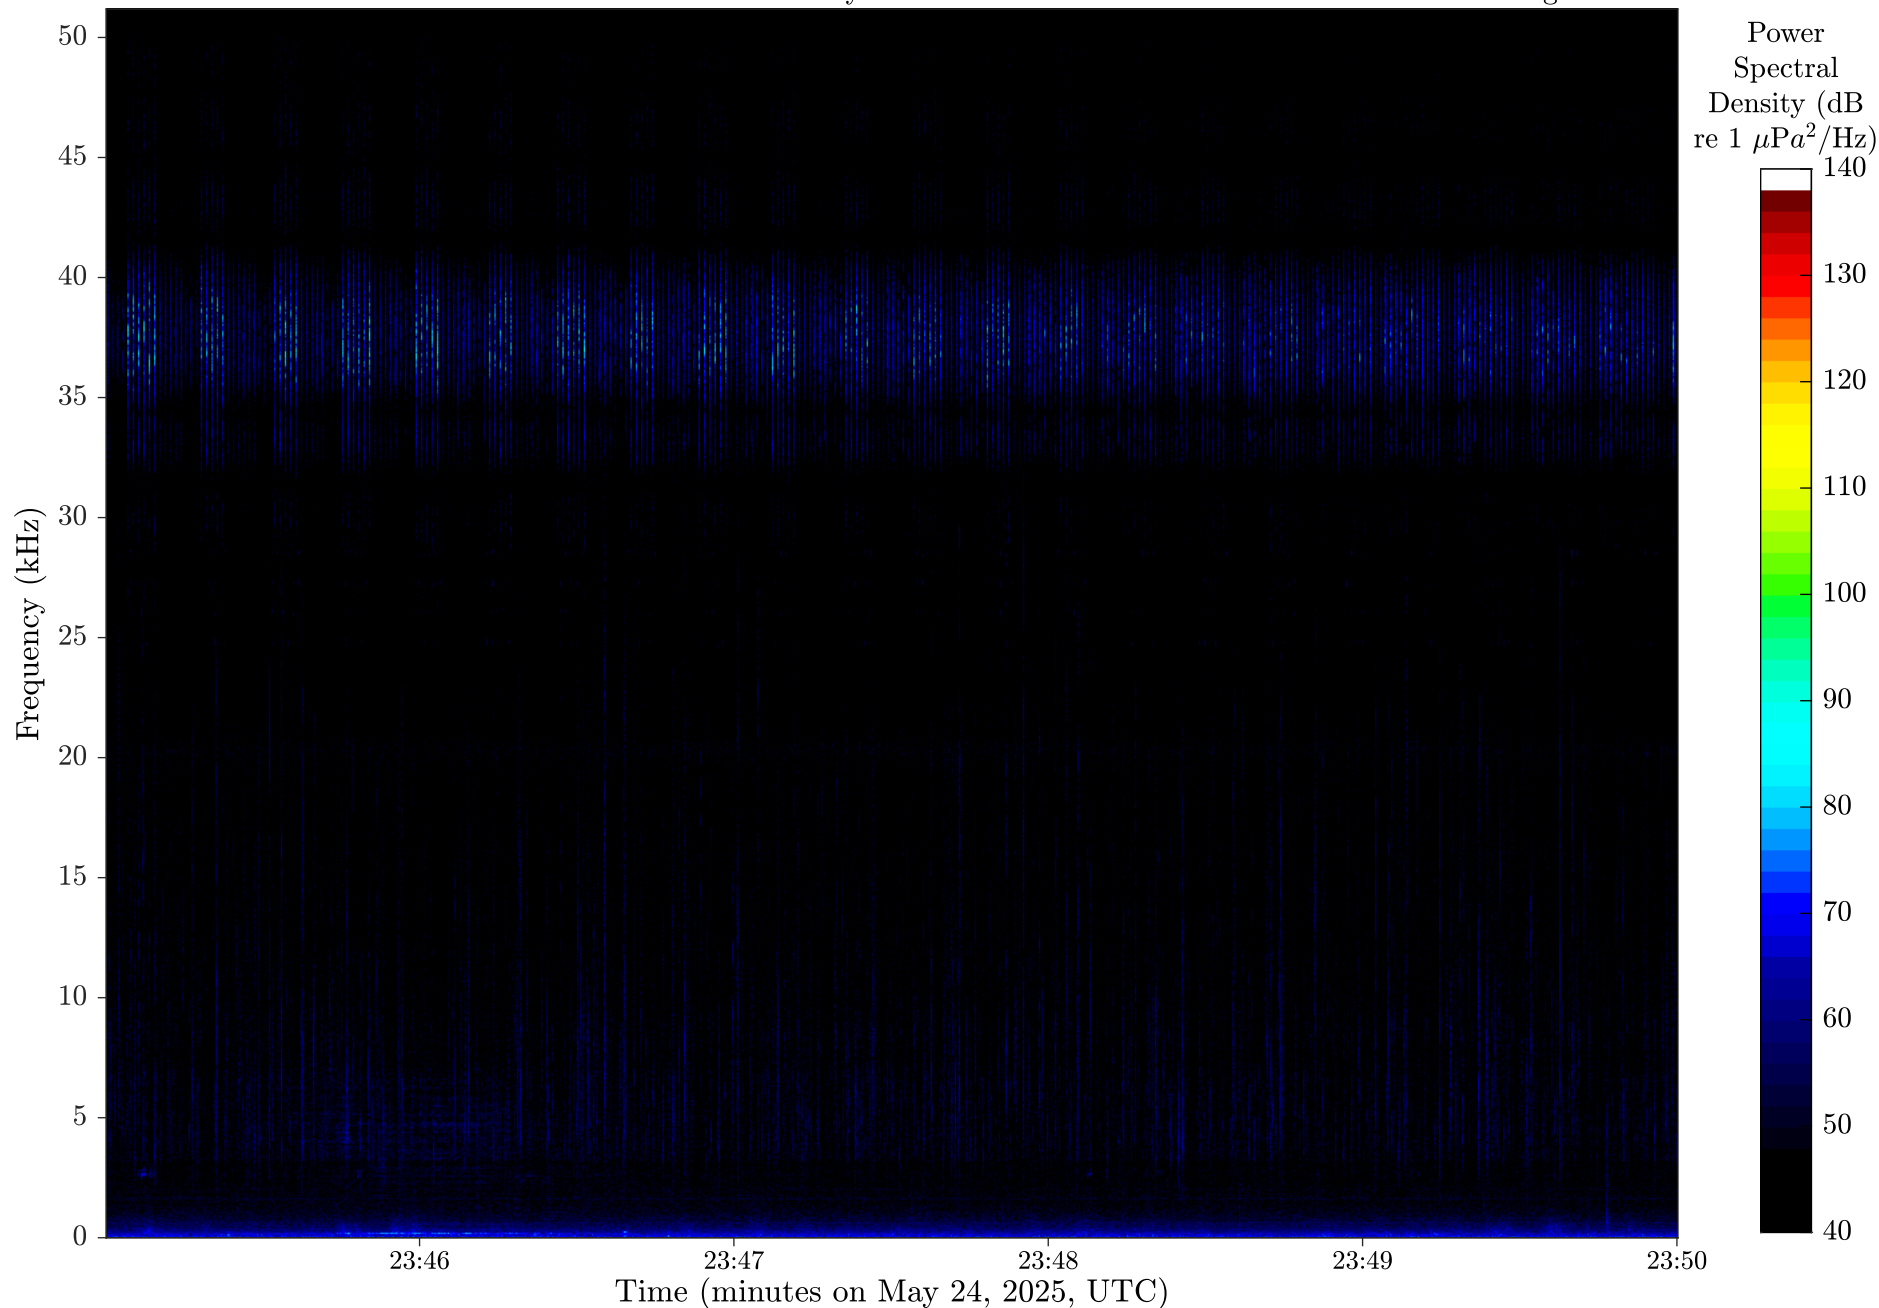

Comments: 34.5 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:57:27 UTC

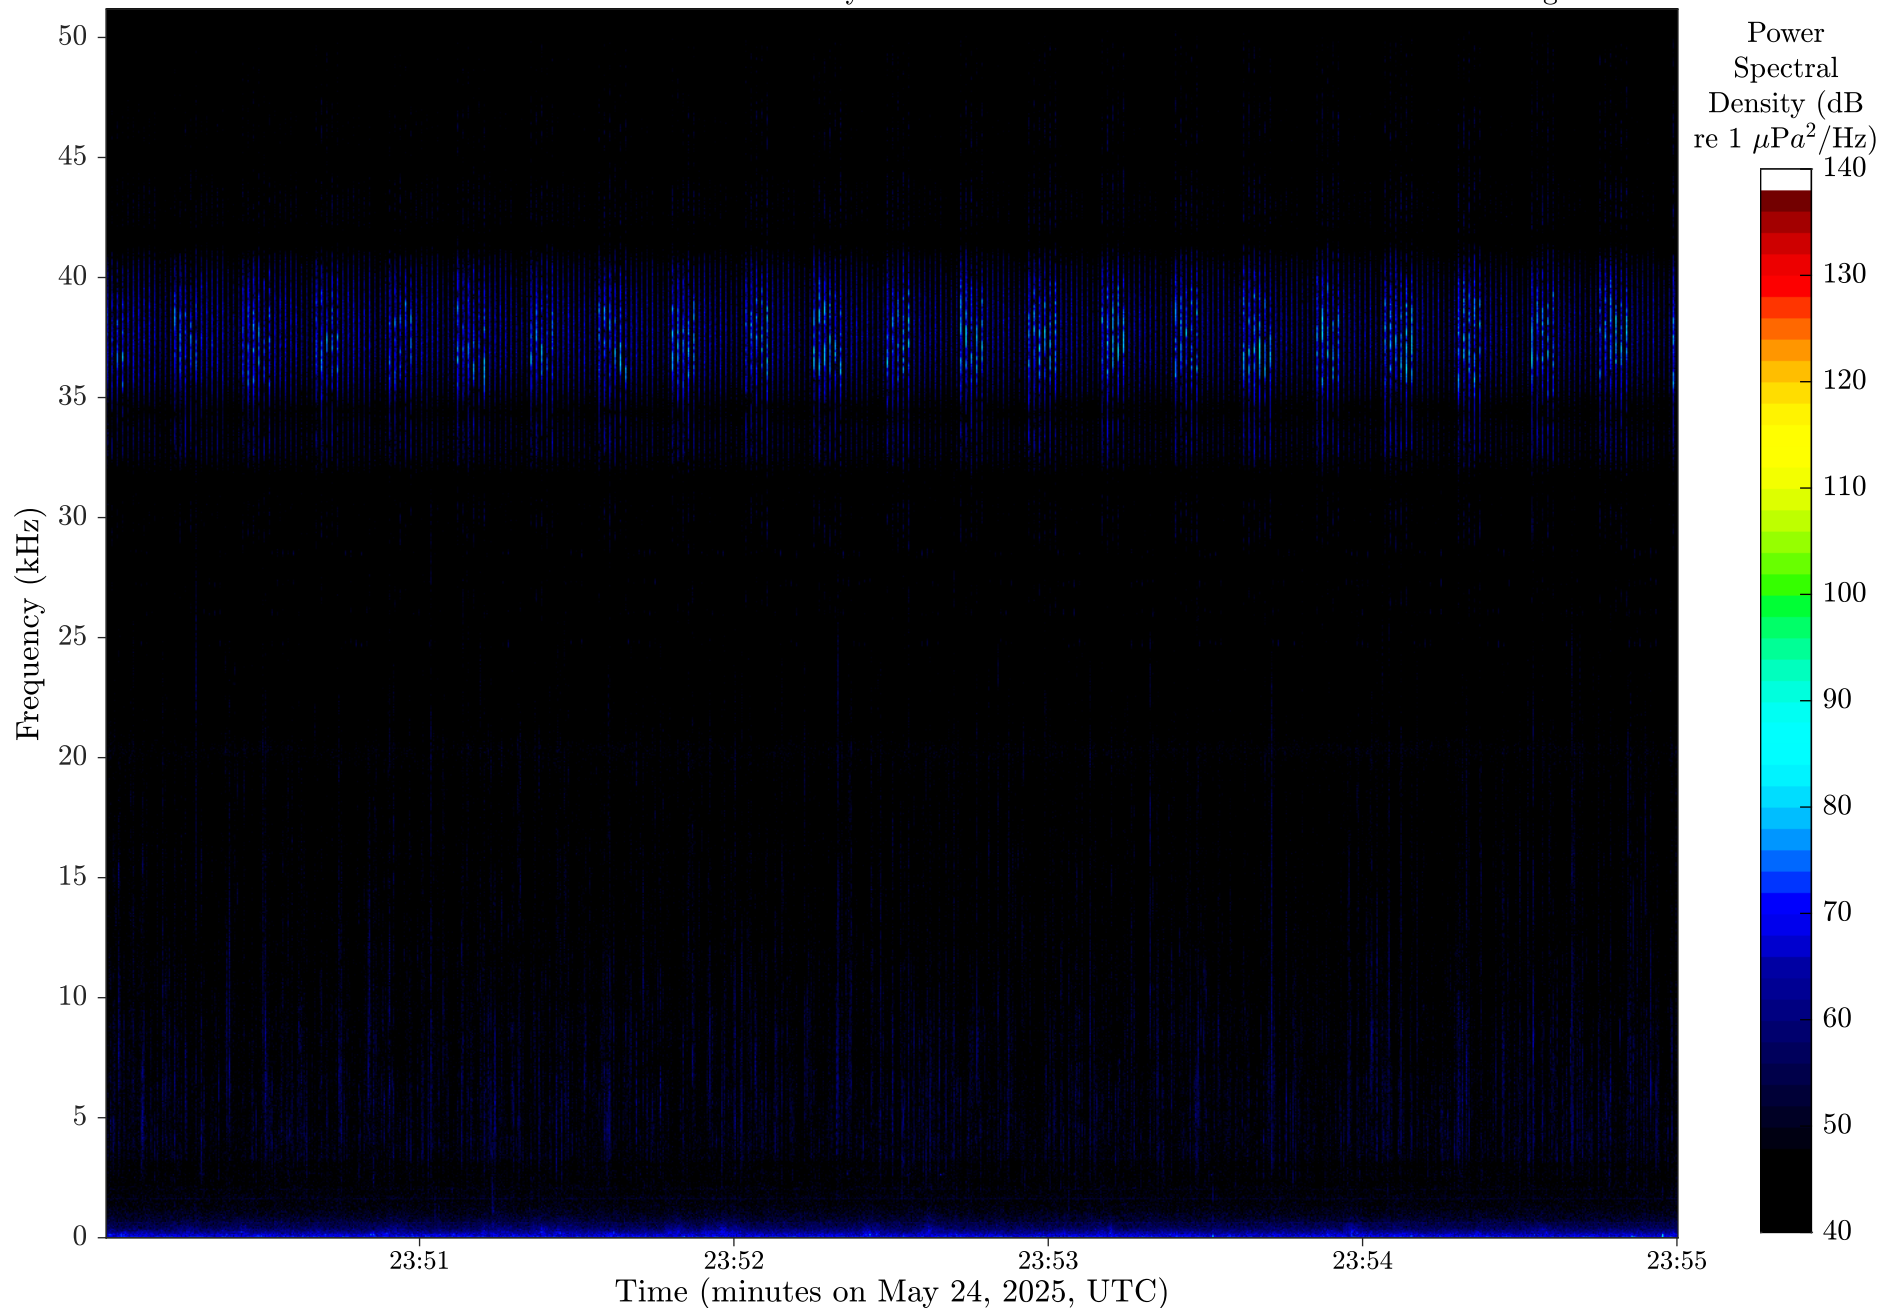

Comments: 34.7 % of spectrogram is less than 40 dB. Hann window with 50% overlap, 12800 samples per FFT window, temporal resolution: 0.05 s, spectral resolution: 10.0 Hz. Sample rate: 128000 Hz. Calibration is applied to each frequency bin individually. Downsampled to 0.10 s, 30.0 Hz resolution.

Plot generated 26-Nov-2025 11:57:34 UTC

